

ภาคผนวก จ  
เอกสารสอบเทียบเครื่องมือ

---



List of Instruments Certification for Environmental Quality Analysis

No.	Instrument/Equipment	Parameter	Manufacturer	Model/Serial No.	Calibrator	Certification No.	Date of Calibration	Due date of Calibration*	Remark
Equipment for Air Quality Analysis									
1	Analytical Balance (Readability 0.1 mg)	ฝุ่นละอองรวม (TSP) ฝุ่นทุกขนาด (Total Dust)	Mettler-Toledo	MS204TS/00 C252436235	National Food Institute, Ministry of Industry, Thailand	2402420-003-01	19 Apr 24	18 Apr 25	-
2	Analytical Balance (Readability 0.001 mg)	Respirable Dust	Mettler-Toledo	XP6 / B322373893	National Food Institute, Ministry of Industry, Thailand	2402420-002-01	19 Apr 24	18 Apr 25	-
3	UV-VIS Spectrophotometer	ก๊าซไนโตรเจนไดออกไซด์ (NOx)	Agilent Technologies	Cary60 G6860A / MY15410009	DQE Services Co.,Ltd.	SP24-018	7 May 24	6 May 25	-
4	Ion Chromatrography (IC)	ไฮโดรเจนคลอไรด์ (HCl), กรดซัลฟิวริก (H <sub>2</sub> SO <sub>4</sub> ), ไอโอดีน (I) คลอรีน (Cl), โซเดียมไฮโปคลอไรท์ ในรูปของคลอรีน (NaOCl as Cl) ไฮโดรเจนซัลไฟด์ (H <sub>2</sub> S)	Dionex	DionexAqionRFC / 220380031	Archemica Lab Co.Ltd.	Qualification Report Anion (ID#1047)	23 Apr 24	22 Apr 25	-
5	Atomic Absorption Spectrophotometer (AAS)	เหล็ก (Fe), นิกเกิล (Ni), โครเมียม (Cr) อะลูมิเนียม (Al) แมกนีเซียมซัลเฟต ในรูปของแมงกนีเซียม	Perkin Elmer	PinAAcle 900F / PFB520031902	Perkin Elmer Co.,Ltd.	Preventive Maintenance Report	14 May 24	13 May 25	-
6	Inductively Coupled Plasma (ICP)	โซเดียมคาร์บอเนต ในรูปของโซเดียมแมงกานีส (Mn)	Agilent Technologies	System ID:G8015A G8015AA / MY18030001	Agilent Technologies (Thailand) Co.,Ltd.		Preventive Maintenance Checklist	4 Nov 24	3 Nov 25
Equipment for Water Quality Analysis									
7	pH Meter	ความเป็นกรด-ด่าง (pH) อุณหภูมิ (Temperature)	Mettler-Toledo	Seven Easy S20 / 1231155210	National Food Institute, Ministry of Industry, Thailand	2401718-001-01	11 Mar 24	10 Mar 25	-
8	pH Meter		Mettler-Toledo	Seven Easy S20 / 1230525212	DKSH (Thailand) Ltd.	C07240167	9 Apr 24	8 Apr 25	-
9	BOD Incubator	ความต้องการออกซิเจนทางชีวเคมี (BOD)	Arco	UC4-1320 / (UAE.WAO.015/2561)	Technology Promotion Association (Thailand-Japan)	24TM303	10 Feb 24	9 Feb 25	-
10	DO Meter		YSI	5100 / 11B101863	Technology Promotion Association (Thailand-Japan)	24TW39	21 Feb 24	20 Feb 25	-
11	Analytical Balance (Readability 0.1 mg)	น้ำมันและไขมัน (Fat Oil and Grease)	Mettler-Toledo	XSR204 / C117635043	Technology Promotion Association (Thailand-Japan)	24MM293	11 May 24	10 May 25	-
Equipment for Water Quality Analysis									
12	Analytical Balance (Readability 0.01 mg)	ของแข็งทั้งหมด (Total Solid) สารแขวนลอย (SS) ปริมาณของแข็งแขวนลอยทั้งหมด (TSS) ปริมาณของแข็งละลายน้ำ (TDS)	Mettler-Toledo	XSR205DU / C210685394	National Food Institute, Ministry of Industry, Thailand	2402283-002-01	2 Apr 24	1 Apr 25	-
13	Hot Air Oven		Memmert	UF55 / B216.1666	National Food Institute, Ministry of Industry, Thailand	2500116-001-01	8 Oct 24	7 Oct 25	-
14	COD Reactor (Heating Block)	ความต้องการออกซิเจนทางเคมี (COD)	Hanna	HI839800 / 1147807	Hanna Instruments (Thailand) Ltd.	HIT-2417-0568	25 Apr 24	24 Apr 25	-
15	Digestor Unit	ทีเคเอ็น (TKN)	FOSS TECATOR	DT2520 / 91794469	National Food Institute, Ministry of Industry, Thailand	2402957-001-01	23 May 24	22 May 25	-
16	Distillation Unit (Kjeldahl Method)		FOSS TECATOR	KT200 / 91790524	FOSS South East Asia	9810	9 Feb 24	7 Feb 25	-
17	Atomic Absorption Spectrophotometer (AAS)	เหล็ก (Fe) นิกเกิล (Ni) โครเมียม (Cr)	Agilent Technologies	System ID:G8432A AA240FS / MY13160001	Thailand Institute of Scientific and Technological Research(TISTR)	MTC.ACL.No 358/67	11 Mar 24	10 Mar 25	-
18	Inductively Coupled Plasma (ICP)	ตะกั่ว (Pb)	Agilent Technologies	System ID:G8015A G8015AA / MY18030001	Agilent Technologies (Thailand) Co.,Ltd.	Preventive Maintenance Checklist	4 Nov 24	3 Nov 25	-

Due Date of Calibration\* : Based on the annual calibration plan. At least 1 time per year.

## Calibration Certificate

**Certificate No.:** 2402420-003-01  
**Client name:** UNITED ANALYST AND ENGINEERING CONSULTANT CO., LTD.  
**Address:** 3 Soi Udomsuk 41, Sukhumvit Road,  
Bangchack, Prakhnong, Bangkok 10260

Page 1 of 3

**Equipment:** Electronic Balance  
**Manufacturer:** METTLER TOLEDO  
**Model:** MS204TS/00  
**Serial No.:** C252436235  
**ID No.:** UAE.AIR.023/2566  
**Order No.:** 2402420  
**Operation No.:** 2402420-003  
**Date of Receipt:** 19 April 2024  
**Date of Calibration:** 19 April 2024

**Calibrated by** Mr.Pheraphat Tuanjit  
Scientist

**Approved by** *P. Jaengkarnkit*  
( Miss Preeyaporn Jaengkarnkit )

Vice President, Department of Laboratory Services  
Responsible for the Technical Management Team

**Date of Issue:** 23 April 2024

The uncertainties are for a confidence probability of approximately 95%

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the National Food Institute.

F-CS-009 Revision: 01 Date: 20-04-65



## Calibration Report

**Certificate No.:** 2402420-003-01

**Equipment:**

Electronic Balance

**Manufacturer:** METTLER TOLEDO

**Model:** MS204TS/00

**Resolution:** 0.0001 g

**Serial No.:** C252436235

**ID No.:** UAE.AIR.023/2566

**Capacity:** 220 g

**Date of Calibration:** 19 April 2024

Page 2 of 3

**Environment Condition:** Ambient Temperature: 21.7 ± 1.5 °C Relative Humidity: 65 ± 6.7 %

**Place of Calibration:** Room 206 Balance Room 2, UNITED ANALYST AND ENGINEERING CONSULTANT CO., LTD.

**Condition of Equipment:** Good Condition

**Condition of This Results of Calibration:**

1. Calibration Method: NFI Method W-MA-001 In-House Method based on UKAS Lab 14 : 2019

2. Reference Standards:

Reference Standard	Model	Serial No.	Calibrated By	Certificate No.	Due Date
Standard Weight Class E2	1-500mg	15880	TCS	M2311181S	28 November 2024
Standard Weight Class E2	1-500g	15882	TCS	M2311182S	28 November 2024

Instrument	Model	Serial No.	Calibrated By	Certificate No.	Due Date
Thermo-Hygro Meter	608-H1	NFI.BTH 019/23	Quality Reborn	QR24-0492	4 March 2025

3. This certification is traceable to SI UNIT

4. This certificate was certified only for the instrument we calibrated.

5. This result of calibration was found accurate as shown on date and place of calibration only.

**Calibration Results:**




**1. Repeatability of Reading:**

Nominal Value ( g )	Standard Deviation of Reading ( g )
100	0.000074
200	0.000074

**2. Off-Center Error:**

A mass of 100 g was placed and moved to various position on pan.

The balance reading obtained is given in the table.



1	2	3	4	5	6	(Maximum Difference)
( g )	( g )	( g )	( g )	( g )	( g )	( g )
100.0005	100.0006	100.0003	100.0006	100.0003	100.0005	0.0002

*P. Jaenghant*  
23 April 2024



## Calibration Report

**Certificate No.:** 2402420-003-01

**Equipment:**

Electronic Balance

**Manufacturer:** METTLER TOLEDO

**Model:** MS204TS/00

**Resolution:** 0.0001 g

**Serial No.:** C252436235

**ID No.:** UAE.AIR.023/2566

**Capacity:** 220 g

**Date of Calibration:** 19 April 2024

Page 3 of 3

**Calibration Results:** (Continued)

**Calibration Range:** 0-200 g

**Calibration Adjustment:** Internal Calibration

### 3. Departure from Nominal Value:

Nominal Value ( g )	Standard Value ( g )	Average Reading ( g )	Correction ( g )	Uncertainty ( ± g )	Coverage Factor k
Unload	0.00000	0.0000	0.0000	0.000094	2.00
0.1	0.10000	0.1000	0.0000	0.000094	2.00
1	0.99998	1.0000	0.0000	0.000097	2.00
5	4.99997	5.0000	0.0000	0.000096	2.00
10	10.00002	10.0000	0.0000	0.00012	2.00
20	20.00003	20.0001	-0.0001	0.00014	2.00
50	49.99998	50.0003	-0.0003	0.00012	2.00
70	70.00000	70.0005	-0.0005	0.00017	2.00
100	99.99997	100.0006	-0.0006	0.00017	2.00
150	149.99994	150.0012	-0.0013	0.00022	2.00
200	200.00001	200.0015	-0.0015	0.00028	2.00

*P. Jaengbanchit*  
23 April 2024

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor  $k$ , providing a level of confidence of approximately 95 %.

----- End -----

F-CS-012 Revision: 01 Date: 20-04-65



## Calibration Certificate

**Certificate No.:** 2402420-002-01  
**Client name:** UNITED ANALYST AND ENGINEERING CONSULTANT CO., LTD.  
**Address:** 3 Soi Udomsuk 41, Sukhumvit Road,  
Bangchack, Prakhonong, Bangkok 10260

Page 1 of 3

**Equipment:** Electronic Balance  
**Manufacturer:** METTLER TOLEDO  
**Model:** XP6  
**Serial No.:** B322373893  
**ID No.:** UAE.AIR.019/2556  
**Order No.:** 2402420  
**Operation No.:** 2402420-002  
**Date of Receipt:** 19 April 2024  
**Date of Calibration:** 19 April 2024

**Calibrated by** Mr.Pheraphat Tuanjit  
Scientist

**Approved by**   
( Miss Preeyaporn Jaengkarnkit )

Vice President, Department of Laboratory Services  
Responsible for the Technical Management Team

**Date of Issue:** 23 April 2024

**The uncertainties are for a confidence probability of approximately 95%**

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the National Food Institute.

F-CS-009 Revision: 01 Date: 20-04-65



## Calibration Report

**Certificate No.:** 2402420-002-01

**Equipment:**

Electronic Balance

**Manufacturer:** METTLER TOLEDO

**Model:** XP6

**Resolution:** 0.000001 g

**Serial No.:** B322373893

**ID No.:** UAE.AIR.019/2556

**Capacity:** 6.1 g

**Date of Calibration:** 19 April 2024

Page 2 of 3

**Environment Condition:** Ambient Temperature: 22.6 ± 1.8 °C Relative Humidity: 48 ± 6.0 %

**Place of Calibration:** Room 206 Balance Room 2, UNITED ANALYST AND ENGINEERING CONSULTANT CO., LTD.

**Condition of Equipment:** Good Condition

**Condition of This Results of Calibration:**

1. Calibration Method: NFI Method W-MA-001 In-House Method based on UKAS Lab 14 : 2019

2. Reference Standards:

Reference Standard	Model	Serial No.	Calibrated By	Certificate No.	Due Date
Standard Weight Class E2	1-500mg	15880	TCS	M2311181S	28 November 2024
Standard Weight Class E2	1-500g	15882	TCS	M2311182S	28 November 2024

Instrument	Model	Serial No.	Calibrated By	Certificate No.	Due Date
Thermo-Hygro Meter	608-H1	NFI.BTH 019/23	Quality Reborn	QR24-0492	4 March 2025

3. This certification is traceable to SI UNIT

4. This certificate was certified only for the instrument we calibrated.

5. This result of calibration was found accurate as shown on date and place of calibration only.

**Calibration Results:**




**1. Repeatability of Reading:**

Nominal Value ( g )	Standard Deviation of Reading ( g )
3	0.00000057
6	0.00000019

**2. Off-Center Error:**

A mass of 2 g was placed and moved to various position on pan.

The balance reading obtained is given in the table.



1	2	3	4	5	6	(Maximum Difference)
( g )	( g )	( g )	( g )	( g )	( g )	( g )
1.999981	1.999983	1.999980	1.999984	1.999983	1.999981	0.000003

F-CS-012 Revision: 01 Date: 20-04-65

P. Jongsakulkit  
23 April 2024



## Calibration Report

**Certificate No.:** 2402420-002-01

**Equipment:**

Electronic Balance

**Manufacturer:** METTLER TOLEDO

**Model:** XP6

**Resolution:** 0.000001 g

**Serial No.:** B322373893

**ID No.:** UAE.AIR.019/2556

**Capacity:** 6.1 g

**Date of Calibration:** 19 April 2024

Page 3 of 3

**Calibration Results:** (Continued)

**Calibration Range:** 0-6 g

**Calibration Adjustment:** Internal Calibration

### 3. Departure from Nominal Value:

Nominal Value ( g )	Standard Value ( g )	Average Reading ( g )	Correction ( g )	Uncertainty ( ± g )	Coverage Factor k
Unload	0.0000000	0.000000	0.000000	0.0000032	2.00
0.01	0.0099970	0.009999	-0.000002	0.0000047	2.00
0.05	0.0500010	0.050003	-0.000002	0.0000048	2.00
0.10	0.1000010	0.100001	0.000000	0.0000069	2.00
0.15	0.1500020	0.150002	0.000000	0.0000083	2.00
0.17	0.1700050	0.170006	-0.000001	0.000012	2.00
0.20	0.1999990	0.200002	-0.000003	0.0000083	2.00
1.50	1.4999750	1.499971	0.000004	0.000027	2.00
3.00	2.9999680	2.999959	0.000009	0.000028	2.00
4.50	4.4999810	4.499967	0.000014	0.000022	2.00
6.00	5.9999490	5.999931	0.000018	0.000032	2.00

*S. Jongsakulkit*  
23 April 2024

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor  $k$ , providing a level of confidence of approximately 95 %.


----- End -----

F-CS-012 Revision: 01 Date: 20-04-65




**CERTIFICATE OF CALIBRATION****Certificate No. :** SP24-018

Page 1 of 5

**Customer :** United Analyst and Engineering Consultant Co.,Ltd. (Head Office)**Address :** 3 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260**Location of calibration :** Laboratory 315**Equipment :** UV-Vis Spectrophotometer**Manufacturer :** Agilent Technologies**Model :** Cary 60**Serial No. :** MY15410009**ID No. :** UAE.WAT.020/2558**Received Date :** 7 May 2024**Calibration Date :** 7 May 2024**Issue Date :** 9 May 2024**Condition Instrument :** Good**Calibrated by :**

( Mr.Tanawut Rittidach )

Technical Manager

**Approved by :**

( Ms. Chonthicha Sangngern )

Quality Manager

The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only.

The measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the DQE Services Co., Ltd.



## REPORT OF CALIBRATION

**Certificate No. :** SP24-018

Page 2 of 5

**Environment Condition :** Ambient Temperature  $25 \pm 5$  °CRelative humidity  $55 \pm 20$  %RH**Calibration method :** In-house method CP-01 Based on ASTM E275-08**Certified Reference Materials :**

Material	Serial No.	Certificate No.	Due date
Absorbance Standard set	25760	115663	25 October 2025
Absorbance Standard set	25757	115638	25 October 2025
Wavelength Standard set	25806	115657	25 October 2025
Wavelength Standard set	25758	115665	25 October 2025

**Traceability :** This certification is traceable to the International System of Unit maintained at National -

Institute of Standards and Technology (NIST) through Sarna Scientific Limited

**Spectral Band Width of UUC :** 1.5 nm.**Scan Speed of UUC :** 60 nm/min**Scan Interval of UUC :** 0.15 nm.**Resolution of UUC :** Photometric 0.0001 Abs.

Wavelength 0.1 nm.

## REPORT OF CALIBRATION

Certificate No. : SP24-018

Page 3 of 5

Calibration Results : Without adjustment

Photometric Accuracy :

Wavelength (nm.)	CRMs Values (Abs)	UUC Reading (Abs)	Correction (Abs)	Uncertainty (Abs)	Coverage factor <i>k</i>
420	0.0000	0.0000	0.0000	0.0028	2.00
	0.5780	0.5747	0.0033	0.0031	2.00
	1.0484	1.0438	0.0046	0.0029	2.00
	2.1876	2.1832	0.0044	0.0080	2.00
440	0.0000	0.0000	0.0000	0.0028	2.00
	0.5595	0.5581	0.0014	0.0034	2.00
	1.0239	1.0231	0.0008	0.0035	2.00
	2.1230	2.1219	0.0011	0.0080	2.00
465	0.0000	0.0000	0.0000	0.0028	2.00
	0.5230	0.5184	0.0046	0.0030	2.00
	0.9633	0.9614	0.0019	0.0029	2.00
	1.9753	1.9731	0.0022	0.0070	2.00
546.1	0.0000	0.0000	0.0000	0.0028	2.00
	0.5181	0.5150	0.0031	0.0031	2.00
	1.0002	0.9964	0.0038	0.0033	2.00
	1.9973	1.9914	0.0059	0.0088	2.00
590	0.0000	0.0000	0.0000	0.0028	2.00
	0.5517	0.5485	0.0032	0.0030	2.00
	1.0803	1.0772	0.0031	0.0030	2.00
	2.0373	2.0293	0.0080	0.0080	2.00
635	0.0000	0.0000	0.0000	0.0028	2.00
	0.5591	0.5565	0.0026	0.0031	2.00
	1.0518	1.0482	0.0036	0.0030	2.00
	1.9274	1.9202	0.0072	0.0079	2.00

## REPORT OF CALIBRATION

Certificate No. : SP24-018

Page 4 of 5

### Photometric Accuracy :

Wavelength (nm.)	CRMs Values (Abs)	UUC Reading (Abs)	Correction (Abs)	Uncertainty (Abs)	Coverage factor <i>k</i>
235	0.0000	0.0000	0.0000	0.0050	2.00
	0.7469	0.7435	0.0034	0.0057	2.00
257	0.0000	0.0000	0.0000	0.0050	2.00
	0.8674	0.8639	0.0035	0.0060	2.00
313	0.0000	0.0000	0.0000	0.0050	2.00
	0.2919	0.2907	0.0012	0.0051	2.00
350	0.0000	0.0000	0.0000	0.0050	2.00
	0.6430	0.6402	0.0028	0.0055	2.00

## REPORT OF CALIBRATION

Certificate No. : SP24-018

Page 5 of 5

### Wavelength Accuracy :

CRMs Values (nm.)	UUC Reading (nm.)	Correction (nm.)	Uncertainty (nm.)	Coverage factor <i>k</i>
241.72	242.0	-0.28	0.18	2.00
279.45	279.5	-0.05	0.18	2.00
287.81	287.9	-0.09	0.18	2.00
334.06	333.9	0.16	0.18	2.00
360.93	360.5	0.43	0.18	2.00
418.59	418.1	0.49	0.18	2.00
445.94	445.6	0.34	0.18	2.00
453.66	453.3	0.36	0.18	2.00
460.02	459.8	0.22	0.18	2.00
536.59	536.0	0.59	0.18	2.00
637.98	638.7	-0.72	0.18	2.00
431.38	430.8	0.58	0.18	2.00
472.50	472.4	0.10	0.18	2.00
513.47	513.7	-0.23	0.18	2.00
528.88	529.1	-0.22	0.18	2.00
573.17	573.5	-0.33	0.18	2.00
585.35	585.2	0.15	0.20	2.00
684.40	685.1	-0.70	0.18	2.00
740.72	741.4	-0.68	0.20	2.00
748.55	749.1	-0.55	0.18	2.00
807.03	807.3	-0.27	0.18	2.00
879.28	879.3	-0.02	0.18	2.00

Remark : - UUC = Unit Under Calibration

- N/A = Not Available

- The result expanded uncertainty of measurement  $U$  is stated as the standard uncertainty of measurement multiplied by the coverage factor  $k$ ,

which for a normal distribution corresponds to a coverage probability of approximately 95%

- \* Indicates non TISI accredited

- End of Certificate -

**เอกสารไม่ควบคุม**  
 FM-708-02 R01 1/11/2021





## Certificate of Calibration

### AquionRFIC : Anion (ID#1047)

This certificate is to verify that instrument below are calibrated

by Archemica Lab Co.,Ltd.

AquionRFIC

S/N : 220380031

AS-DV

S/N : 220360045

for  
**United Analyst and Engineering Consultant Co.,Ltd.**

ARCHEMICA LAB  
บริษัท อาร์เคมีกา แล็บ จำกัด  
ARCHEMICA LAB CO.,LTD.

Operator Signature : K. Channarong

Date : Apr 23, 2024

(Mr.Channarong Khiao-Un)

Test Engineer

เอกสารไม่ควบคุม



# **Qualification Report**

**PM Check list,CM\_OQ and PQ**

**AquionRFIC : Anion (ID#1047)**

**Aquion : Cation (ID#1048)**

**For**

**United Analyst Engineering Conslutand Co.,Ltd.**

**(Validate System 2024)**

# **PM** Anion ID#1047

---

## **Preventive Maintenance Check List**



## Dionex Ion Chromatography Preventive Maintenance Report

Customer Organization	Name/ Department
United Analyst and Engineering Consultant Co.,Ltd.	Khun.Suwan Kongthong / Lab
Engineer	Date
Mr.Channarong Khiao-Un	23-24/Apr/2024

### Instrument Detail

Instrument Model	Application
AquionRFIC	Anion
Instrument components	Serial Number
AquionRFIC	220380031
AS-DV	220360045

### Consumable Detail

Columns	Guard Columns	Suppressors	Concentrators	Etc.
AS18	AG18	ADRS-600	-	EGC III KOH
				CR-ATC

**Remark:** แนะนำเปลี่ยน Column, Guard Column และ Suppressor เนื่องจาก peak shift และ tail

Perform By Archemica

  
บริษัท อาร์เคมีกา แล็บ จำกัด  
ARCHEMICA LAB CO.,LTD

K. Channarong Khiao-Un  
Archemica  
Date 23/Apr/2024

Suwan Kongthong  
Customer  
Date 23/Apr/2024

เอกสารไม่ควบคุม

## General ICS Maintenance Checklist

No.	Description	Result			
<b>Power on &amp; Connection</b>		<b>Checked</b>	<b>Cleaned</b>	<b>Replaced</b>	<b>N.A.</b>
1	Instrument power on	<input checked="" type="checkbox"/>	-	-	<input type="checkbox"/>
2	Instrument connection	<input checked="" type="checkbox"/>	-	-	<input type="checkbox"/>
<b>Injection Valve Rebuild</b>		<b>Checked</b>	<b>Cleaned</b>	<b>Replaced</b>	<b>N.A.</b>
3	Rebuilt injection valve 6 port	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
4	- Rotor seal	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
5	- Stator face	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
<b>(Optional) Auxiliary Valve Rebuild</b>		<b>Checked</b>	<b>Cleaned</b>	<b>Replaced</b>	<b>N.A.</b>
6	Rebuilt auxiliary valve - port	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>
7	- Rotor seal	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>
8	- Stator face	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>
<b>Check Valve Cartridge</b>		<b>Checked</b>	<b>Cleaned</b>	<b>Replaced</b>	<b>N.A.</b>
9	Inlet check valve assembly	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
10	Outlet check valve assembly	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
11	Verified correct flow orientation	<input checked="" type="checkbox"/>	-	-	<input type="checkbox"/>
<b>Pump Piston Rinse Seal, Piston Seal and Piston</b>		<b>Checked</b>	<b>Cleaned</b>	<b>Replaced</b>	<b>N.A.</b>
12	Piston rinse seal in <i>primary</i> pump head	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
13	Piston seal in <i>primary</i> pump head	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
14	Piston in <i>primary</i> pump head	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
15	Piston rinse seal in <i>secondary</i> pump head	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
16	Piston seal in <i>secondary</i> pump head	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
17	Piston in <i>secondary</i> pump head	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
<b>Waste Valve and Priming Valve</b>		<b>Checked</b>	<b>Cleaned</b>	<b>Replaced</b>	<b>N.A.</b>
18	Waste valve	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
19	Priming valve	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
<b>Cell Detector</b>		<b>Checked</b>	<b>Cleaned</b>	<b>Replaced</b>	<b>N.A.</b>
20	Check conductivity cell	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
21	Check electrochemical cell	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>
22	- Working electrode	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>
23	- Reference electrode	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>
24	- Gasket	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>
25	- Cell body	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>
<b>Other</b>		<b>Checked</b>	<b>Cleaned</b>	<b>Replaced</b>	<b>N.A.</b>
26	Sample Loop	Size 25 uL	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>
27	End-line filter		<input checked="" type="checkbox"/>	-	<input type="checkbox"/>
28	Leak sensor		<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
29	Lubricate pump mechanic		<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>
30	Reconnected liquid lines to the valve		<input checked="" type="checkbox"/>	-	<input type="checkbox"/>
31	Reconnected liquid lines to pump heads		<input checked="" type="checkbox"/>	-	<input type="checkbox"/>
32	Primed pump		<input checked="" type="checkbox"/>	-	<input type="checkbox"/>
33	Checked pump for leaks		<input checked="" type="checkbox"/>	-	<input type="checkbox"/>
34	Checked gas for leaks		<input checked="" type="checkbox"/>	-	<input type="checkbox"/>

**AS-DV Autosampler Preventive Maintenance Checklist**

Model	Serial number	Firmware Version
<input checked="" type="checkbox"/> AS-DV	220360045	1.6.0

No.	Description	Result			
Power on & Connection		Checked	Cleaned	Replaced	N.A
1.	AS-DV power on	<input checked="" type="checkbox"/>	-	-	<input type="checkbox"/>
2.	AS-DV connection	<input checked="" type="checkbox"/>	-	-	<input type="checkbox"/>
Sampling Tip		Checked	Cleaned	Replaced	N.A
3.	Sampling needle	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
4.	Sampling tubing (Transfer line)	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
5.	Reconnect sampling needle & tubing	<input checked="" type="checkbox"/>	-	-	<input type="checkbox"/>
Other		Checked	Cleaned	Replaced	N.A
6.	Check carousel movement	<input checked="" type="checkbox"/>	-	-	<input type="checkbox"/>
7.	Check needle movement	<input checked="" type="checkbox"/>	-	-	<input type="checkbox"/>
8.	Lubricate needle drive	<input type="checkbox"/>	<input checked="" type="checkbox"/> Lubricated	-	<input type="checkbox"/>
9.	AS-DV cover	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
(Optional) High Pressure Valve		Checked	Cleaned	Replaced	N.A
10.	High pressure valve - Port	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>
11.	- Rotor seal	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>
12.	- Stator face	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>
13.	- Reconnected liquid line to the valve	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>

<b>Others / comments:</b>



# **PM** Cation ID#1048

---

## **Preventive Maintenance Check List**



## Dionex Ion Chromatography Preventive Maintenance Report

Customer Organization	Name/ Department
United Analyst and Engineering Consultant Co.,Ltd.	Khun.Suwan Kongthong / Lab
Engineer	Date
Mr.Channarong Khiao-Un	23-24/Apr/2024

### Instrument Detail

Instrument Model	Application
Aquion	Cation
Instrument components	Serial Number
Aquion	220340349


### Consumable Detail

Columns	Guard Columns	Suppressors	Concentrators	Etc.
CS12A	CG12A	CDER-600	-	-
<b>Remark:</b> แนะนำให้เปิดเครื่องใช้งานบ่อยๆ, System ยังไม่ได้ใช้งาน				

Perform By Archemica

  
Archemica  
Date 23/Apr/2024



  
Customer  
Date 23/Apr/2024

เอกสารไม่ควบคุม

## General ICS Maintenance Checklist

No.	Description		Result			
Power on & Connection			Checked	Cleaned	Replaced	N.A.
1	Instrument power on		<input checked="" type="checkbox"/>	-	-	<input type="checkbox"/>
2	Instrument connection		<input checked="" type="checkbox"/>	-	-	<input type="checkbox"/>
Injection Valve Rebuild			Checked	Cleaned	Replaced	N.A.
3	Rebuilt injection valve 6 port		<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
4	-	Rotor seal	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
5	-	Stator face	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
(Optional) Auxiliary Valve Rebuild			Checked	Cleaned	Replaced	N.A.
6	Rebuilt auxiliary valve - port		<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>
7	-	Rotor seal	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>
8	-	Stator face	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>
Check Valve Cartridge			Checked	Cleaned	Replaced	N.A.
9	Inlet check valve assembly		<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
10	Outlet check valve assembly		<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
11	Verified correct flow orientation		<input checked="" type="checkbox"/>	-	-	<input type="checkbox"/>
Pump Piston Rinse Seal Piston Seal and Piston			Checked	Cleaned	Replaced	N.A.
12	Piston rinse seal in <i>primary</i> pump head		<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
13	Piston seal in <i>primary</i> pump head		<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
14	Piston in <i>primary</i> pump head		<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
15	Piston rinse seal in <i>secondary</i> pump head		<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
16	Piston seal in <i>secondary</i> pump head		<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
17	Piston in <i>secondary</i> pump head		<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Waste Valve and Priming Valve			Checked	Cleaned	Replaced	N.A.
18	Waste valve		<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
19	Priming valve		<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Cell Detector			Checked	Cleaned	Replaced	N.A.
20	Check conductivity cell		<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
21	Check electrochemical cell		<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>
22	-	Working electrode	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>
23	-	Reference electrode	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>
24	-	Gasket	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>
25	-	Cell body	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>
Other			Checked	Cleaned	Replaced	N.A.
26	Sample Loop	Size 25 uL	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
27	End-line filter		<input type="checkbox"/>	-	<input type="checkbox"/>	<input type="checkbox"/>
28	Leak sensor		<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
29	Lubricate pump mechanic		<input type="checkbox"/>	<input type="checkbox"/> Lubricated	-	<input type="checkbox"/>
30	Reconnected liquid lines to the valve		<input checked="" type="checkbox"/>	-	-	<input type="checkbox"/>
31	Reconnected liquid lines to pump heads		<input checked="" type="checkbox"/>	-	-	<input type="checkbox"/>
32	Primed pump		<input checked="" type="checkbox"/>	-	-	<input type="checkbox"/>
33	Checked pump for leaks		<input checked="" type="checkbox"/>	-	-	<input type="checkbox"/>
34	Checked gas for leaks		<input checked="" type="checkbox"/>	-	-	<input type="checkbox"/>

# CM OQ

---

**Chromeleon**

**Operation Qualification**

**ThermoFisher**  
S C I E N T I F I C  
**Chromeleon Operational Qualification**

**General Information**

	Computer Name	Version Number:
Instrument Controller:	DESKTOP-C4FS3L7	7.3.1 Build 6535
Client:	DESKTOP-C4FS3L7	7.3.1.6535
Operator:	Mr.Channarong Khiao-Un	

**Overall Test Result:**      ***Passed***

**Comparison Format:**

All Parameters:	Significant Digits:	10
-----------------	---------------------	----



\_\_\_\_\_  
Reviewer's Signature // Date

K. CHANNARONG 23/Apr/2024  
\_\_\_\_\_  
Operator's Signature // Date

**เอกสารไม่ควบคุม**





Chromeleon Operational Qualification, Part 1  
Verification of Selected Results

Detection Algorithm: Cobra  
Calibration Type: Lin, WithOffset  
Evaluation Type: Area  
Standard Method: External  
Calibration Mode: Total

Report Variable	Peak Name	Status
Offset (c0)	Acetanilide	ok
	Acetophenone	ok
	Propiophenone	ok
Slope (c1)	Acetanilide	ok
	Acetophenone	ok
	Propiophenone	ok
Correlation Coeffi.	Acetanilide	ok
	Acetophenone	ok
	Propiophenone	ok
Variance	Acetanilide	ok
	Acetophenone	ok
	Propiophenone	ok
Std. Deviation	Acetanilide	ok
	Acetophenone	ok
	Propiophenone	ok
Rel. Std. Dev.	Acetanilide	ok
	Acetophenone	ok
	Propiophenone	ok
Variance Coeff.	Acetanilide	ok
	Acetophenone	ok
	Propiophenone	ok

**ThermoFisher**  
S C I E N T I F I C

**Chromeleon Operational Qualification, Part 1**  
**Verification of Selected Results**

<i>Report Variable</i>	<i>Peak Name</i>	<i>Status</i>
Calibration Point X	Acetanilide	ok
	Acetophenone	ok
	Propiophenone	ok
Calibration Point Y	Acetanilide	ok
	Acetophenone	ok
	Propiophenone	ok
Amount [ng]	Acetanilide	ok
	Acetophenone	ok
	Propiophenone	ok
Resolution (EP)	Acetanilide	ok
	Acetophenone	ok
Resolution (USP)	Acetanilide	ok
	Acetophenone	ok
Peak Asymmetry (EP/USP)	Acetanilide	ok
	Acetophenone	ok
	Propiophenone	ok
Peak Asymmetry (AIA)	Acetanilide	ok
	Acetophenone	ok
	Propiophenone	ok



Chromeleon Operational Qualification, Part 1  
Verification of Selected Results

<i>Report Variable</i>	<i>Peak Name</i>	<i>Status</i>
Theoretical Plates (EP)	Acetanilide	ok
	Acetophenone	ok
	Propiophenone	ok
Theoretical Plates (USP)	Acetanilide	ok
	Acetophenone	ok
	Propiophenone	ok
Theoretical Plates (JP)	Acetanilide	ok
	Acetophenone	ok
	Propiophenone	ok

Test Result: Passed



Chromeleon Operational Qualification, Part 2

Most Frequently Used Parameters: Comparison with Expected Results

Detection Algorithm: Cobra  
Calibration Type: Lin, WithOffset  
Evaluation Type: Area  
Standard Method: External  
Calibration Mode: Total

Variable Category	Report Variable	Peak Name	Status
Injection	No.		ok
	Name		ok
	Type		ok
	Position		ok
	Status		ok
	Volume		ok
	Dilution Factor		ok
	Weight		ok
	IntStd		ok
	InstrumentMethod		ok
	ProcessingMethod		ok
Chromatogram	Channel		ok
	No. of Peaks		ok
	Chromatogram Start Time		ok
	Signal Min.		ok
	Signal Max.		ok
	Unit		ok
	Noise		ok
Peak Results	No.	Acetanilide	ok
	No.	Acetophenone	ok
	No.	Propiophenone	ok
	Peak Name	Acetanilide	ok
	Peak Name	Acetophenone	ok
	Peak Name	Propiophenone	ok
	Ret.Time	Acetanilide	ok
	Ret.Time	Acetophenone	ok
	Ret.Time	Propiophenone	ok

# ThermoFisher SCIENTIFIC

## Chromeleon Operational Qualification, Part 2

### Most Frequently Used Parameters: Comparison with Expected Results

<u>Variable Category</u>	<u>Report Variable</u>	<u>Peak Name</u>	<u>Status</u>
Peak Results	Abs.Ret.Dev.	Acetanilide	ok
	Ret.Dev.(abs)	Acetophenone	ok
	Ret.Dev.(abs)	Propiophenone	ok
	Rel.Ret.Dev.	Acetanilide	ok
	Ret.Dev.(rel)	Acetophenone	ok
	Ret.Dev.(rel)	Propiophenone	ok
	Area	Acetanilide	ok
	Area	Acetophenone	ok
	Area	Propiophenone	ok
	Rel.Area	Acetanilide	ok
	Rel.Area (Total)	Acetophenone	ok
	Rel.Area (Total)	Propiophenone	ok
	Height	Acetanilide	ok
	Height	Acetophenone	ok
	Height	Propiophenone	ok
	Rel.Height (Total)	Acetanilide	ok
	Rel.Height (Total)	Acetophenone	ok
	Rel.Height (Total)	Propiophenone	ok
	Amount	Acetanilide	ok
	Amount	Acetophenone	ok
	Amount	Propiophenone	ok
	Concentration	Acetanilide	ok
	Concentration	Acetophenone	ok
	Concentration	Propiophenone	ok
	Rel.Amount	Acetanilide	ok
	Rel.Amount	Acetophenone	ok
	Rel.Amount	Propiophenone	ok
	Peak Width (0%)	Acetanilide	ok
	Peak Width (0%)	Acetophenone	ok
	Peak Width (0%)	Propiophenone	ok
	Peak Width (5%)	Acetanilide	ok
	Peak Width (5%)	Acetophenone	ok
	Peak Width (5%)	Propiophenone	ok
	Peak Width (10%)	Acetanilide	ok
	Peak Width (10%)	Acetophenone	ok
	Peak Width (10%)	Propiophenone	ok



# ThermoFisher SCIENTIFIC

## Chromeleon Operational Qualification, Part 2

### Most Frequently Used Parameters: Comparison with Expected Results

<i>Variable Category</i>	<i>Report Variable</i>	<i>Peak Name</i>	<i>Status</i>
Peak Results	Peak Width (50%)	Acetanilide	ok
	Peak Width (50%)	Acetophenone	ok
	Peak Width (50%)	Propiophenone	ok
	Left Width (0%)	Acetanilide	ok
	Left Width (0%)	Acetophenone	ok
	Left Width (0%)	Propiophenone	ok
	Right Width (0%)	Acetanilide	ok
	Right Width (0%)	Acetophenone	ok
	Right Width (0%)	Propiophenone	ok
	Peak Start	Acetanilide	ok
	Peak Start	Acetophenone	ok
	Peak Start	Propiophenone	ok
	Peak Stop	Acetanilide	ok
	Peak Stop	Acetophenone	ok
	Peak Stop	Propiophenone	ok
	Peak Start Value	Acetanilide	ok
	Peak Start Value	Acetophenone	ok
	Peak Start Value	Propiophenone	ok
	Peak Stop Value	Acetanilide	ok
	Peak Stop Value	Acetophenone	ok
	Peak Stop Value	Propiophenone	ok
	BL-Value Peak Start	Acetanilide	ok
	BL-Value Peak Start	Acetophenone	ok
	BL-Value Peak Start	Propiophenone	ok
	BL-Value Peak Stop	Acetanilide	ok
	BL-Value Peak Stop	Acetophenone	ok
	BL-Value Peak Stop	Propiophenone	ok
	Type	Acetanilide	ok
	Type	Acetophenone	ok
	Type	Propiophenone	ok
	Resolution (EP)	Acetanilide	ok
	Resolution(EP)	Acetophenone	ok
	Resolution(USP)	Acetanilide	ok
	Resolution(USP)	Acetophenone	ok
	Asymmetry(EP)	Acetanilide	ok
	Asymmetry(EP)	Acetophenone	ok
	Asymmetry(EP)	Propiophenone	ok

# ThermoFisher SCIENTIFIC

## Chromeleon Operational Qualification, Part 2

### Most Frequently Used Parameters: Comparison with Expected Results

<i>Variable Category</i>	<i>Report Variable</i>	<i>Peak Name</i>	<i>Status</i>
Peak Results	Asymmetry(AIA)	Acetanilide	ok
	Asymmetry(AIA)	Acetophenone	ok
	Asymmetry(AIA)	Propiophenone	ok
	Theor. Plates(EP)	Acetanilide	ok
	Theor. Plates(EP)	Acetophenone	ok
	Theor. Plates(EP)	Propiophenone	ok
	Theor. Plates(USP)	Acetanilide	ok
	Theor. Plates(USP)	Acetophenone	ok
	Theor. Plates(USP)	Propiophenone	ok
	Theor. Plates (JP)	Acetanilide	ok
	Theor. Plates(JP)	Acetophenone	ok
	Theor. Plates(JP)	Propiophenone	ok
Peak Calibration	Cal.Mode	Acetanilide	ok
	Cal.Mode	Acetophenone	ok
	Cal.Mode	Propiophenone	ok
	Cal.Type	Acetanilide	ok
	Cal.Type	Acetophenone	ok
	Cal.Type	Propiophenone	ok
	Weights	Acetanilide	ok
	Weights	Acetophenone	ok
	Weights	Propiophenone	ok
	Calibr. Coefficient C0	Acetanilide	ok
	Calibr. Coefficient C0	Acetophenone	ok
	Calibr. Coefficient C0	Propiophenone	ok
	Calibr. Coefficient C1	Acetanilide	ok
	Calibr. Coefficient C1	Acetophenone	ok
	Calibr. Coefficient C1	Propiophenone	ok
	RF-Value	Acetanilide	ok
	RF-Value	Acetophenone	ok
	RF-Value	Propiophenone	ok
	No. of Points	Acetanilide	ok
	No. of Points	Acetophenone	ok

# ThermoFisher SCIENTIFIC

## Chromeleon Operational Qualification, Part 2

### Most Frequently Used Parameters: Comparison with Expected Results

<i>Variable Category</i>	<i>Report Variable</i>	<i>Peak Name</i>	<i>Status</i>
Peak Calibration	No. of Points	Propiophenone	ok
	No. of Points(disabled)	Acetanilide	ok
	No. of Points(disabled)	Acetophenone	ok
	No. of Points(disabled)	Propiophenone	ok
	Variance	Acetanilide	ok
	Variance	Acetophenone	ok
	Variance	Propiophenone	ok
	Var.Coeff	Acetanilide	ok
	Var.Coeff	Acetophenone	ok
	Var.Coeff	Propiophenone	ok
	Std.Dev.	Acetanilide	ok
	Std.Dev.	Acetophenone	ok
	Std.Dev.	Propiophenone	ok
	Rel.Std.Dev.	Acetanilide	ok
	Rel.Std.Dev.	Acetophenone	ok
	Rel.Std.Dev.	Propiophenone	ok
	Corr.Coeff.	Acetanilide	ok
	Corr.Coeff.	Acetophenone	ok
	Corr.Coeff.	Propiophenone	ok
	R-Square	Acetanilide	ok
	R-Square	Acetophenone	ok
	R-Square	Propiophenone	ok
	Adj. R-Square	Acetanilide	ok
	Adj. R-Square	Acetophenone	ok
	Adj. R-Square	Propiophenone	ok
	X	Acetanilide	ok
	X	Acetophenone	ok
	X	Propiophenone	ok
	Y	Acetanilide	ok
	Y	Acetophenone	ok
	Y	Propiophenone	ok
	W	Acetanilide	ok
	W	Acetophenone	ok
	W	Propiophenone	ok
	F(X)	Acetanilide	ok
	F(X)	Acetophenone	ok
	F(X)	Propiophenone	ok



Chromeleon Operational Qualification, Part 2

Most Frequently Used Parameters: Comparison with Expected Results

<i>Variable Category</i>	<i>Report Variable</i>	<i>Peak Name</i>	<i>Status</i>
Peak Calibration	Residual for Cal.Point X	Acetanilide	ok
	Residual for Cal.Point X	Acetophenone	ok
	Residual for Cal.Point X	Propiophenone	ok
	Calibration Point Status	Acetanilide	ok
	Calibration Point Status	Acetophenone	ok
	Calibration Point Status	Propiophenone	ok
	Amount	Acetanilide	ok
	Amount	Acetophenone	ok
	Amount	Propiophenone	ok
Component	Cal.Type	Acetanilide	ok
	Peak Type	Acetanilide	ok
	Left Limit	Acetophenone	ok
	Right Limit	Acetanilide	ok
	Group	Acetanilide	ok
	Factor	Acetophenone	ok
	Amount	Acetanilide	ok
	Conc.Unit	Acetophenone	ok



**Chromeleon Operational Qualification, Part 2**  
**Most Frequently Used Parameters: Comparison with Expected Results**

<i>Variable Category</i>	<i>Report Variable</i>	<i>Peak Name</i>	<i>Status</i>
Peak Purity	PPI	Acetanilide	ok
	PPI	Acetophenone	ok
	PPI	Propiophenone	ok
	RSD PPI	Acetanilide	ok
	RSD PPI	Acetophenone	ok
	RSD PPI	Propiophenone	ok
	Match	Acetanilide	ok
	Match	Acetophenone	ok
	Match	Propiophenone	ok
	RSD Match	Acetanilide	ok
	RSD Match	Acetophenone	ok
	RSD Match	Propiophenone	ok
	Rel.Max at	Acetanilide	ok
	Rel.Max at	Acetophenone	ok
	Rel.Max at	Propiophenone	ok

**Test Result:**      **Passed**





Chromeleon Operational Qualification, Part 3  
System Suitability Test: Comparison with Expected Results

Variable Category	Report Variable	Status
System Suitability Test Case	Number	ok
	Name	ok
	Inj.Condition	ok
	Eval. Formula	ok
	Operator	ok
	Statistics	ok
	Rounding	ok
	MinimumNumberOfInjections	ok
	MaximumNumberOfInjections	ok
	Channel	ok
	Peak	ok
	Ref. Value Formula 1	ok
	Ref. Value Formula 2	ok
	N.A.	ok
System Suitability Test Case Result	Inj. Eval. Result	ok
	Eval. Result	ok
	Peak Result	ok
	Injection Condition Result	ok
	Ref. Value 1	ok
	Ref. Value 2	ok
	Result	ok
	Message	ok
	Average	ok
	Count	ok
	Maximum	ok
	Minimum	ok
	Range	ok
	Rel. Range	ok
	Rel. Std. Dev.	ok
	Std. Dev.	ok
	Sum	ok

Test Result: Passed

Chromeleon

Part 1 - Verification of Selected Results	PASS
Part 2 - Most Frequently Used Parameters: Comparison with Expected Results	PASS
Part 3 - System Suitability Test: comparison with Expected Results	PASS



OVERALL TEST RESULT: PASS

บริษัท อาร์เคมีกา แล็บ จำกัด  
ARCHEMICA LAB CO.,LTD.

Field Service Representative Signature:	Customer Signature:
	
Date: 23/Apr/2024	Date: 23/Apr/2024

เอกสารไม่ควบคุม

# **PQ** Anion ID#1047

---

## **Performance Qualification**

Test Equipment


Equipment	Manufacturer	Model	Serial Number	Cal/Ver Date	Good Until
Multimeter	Fluke	289	27970244	N/A	N/A
Thermocouple	Fluke	K-Type	27970244	N/A	N/A
Balance	Mettler Toledo	AB204-S	1129361010	N/A	N/A
IC Qualification	Thermo Scientific	Test Box	21379153	N/A	N/A
N/A	N/A	N/A	N/A	N/A	N/A

Standards/Chemicals

Description	Manufacturer	Concentration	Part Number	Lot Number	Expiration Date
Nitrate	Thermo Scientific	5 ppm	060254	231226	Dec-2024
Nitrate	Thermo Scientific	10 ppm	060254	231226	Dec-2024
Nitrate	Thermo Scientific	25 ppm	060254	231226	Dec-2024
Nitrate	Thermo Scientific	50 ppm	060254	231226	Dec-2024
Nitrate	Thermo Scientific	100 ppm	060254	231226	Dec-2024
Nitrate	Thermo Scientific	1000 ppm	060254	231226	Dec-2024
N/A	N/A	N/A	N/A	N/A	N/A
N/A	N/A	N/A	N/A	N/A	N/A
N/A	N/A	N/A	N/A	N/A	N/A
N/A	N/A	N/A	N/A	N/A	N/A



Field Service Representative Signature:	Customer Signature:
<i>K. Khamrath</i>	<i>Samran</i>
Date: 23/Apr/2024	Date: 23/Apr/2024

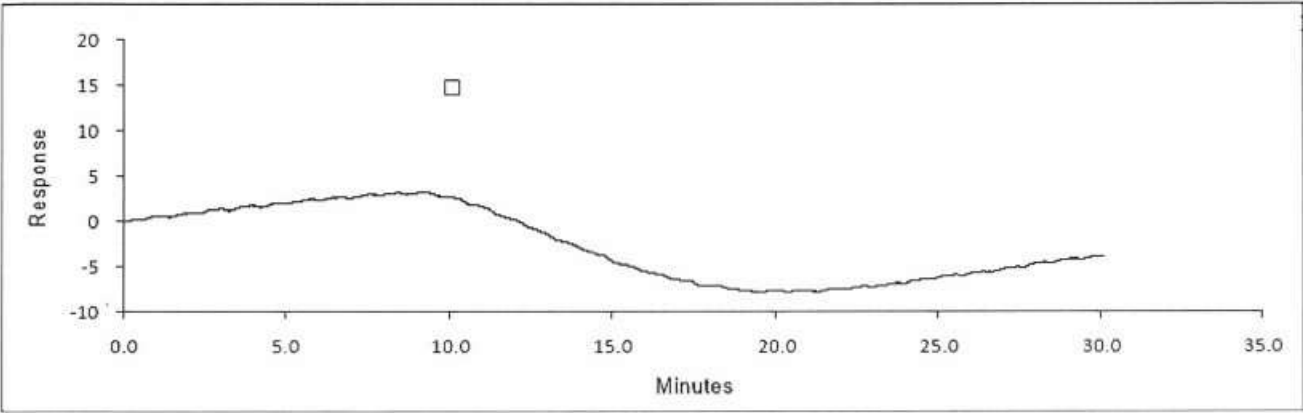

Information

System Name	Aquion RFIC
Detector SN	220360045
Data Path	chrom:///desktop-c4fs3l7/ChromeleonLocal/Archemica/Service Contract/Validate 2024/1PM1PQ 23-04-24/Anion/IC OQ.seq/278.smp/ECD_1.channel

Noise and Drift

Test	Measured (nS)	OQ Limit (nS)	Result	Conversion Factor
Noise	1.1 nS	$\leq 2.0$ nS	PASS	1000
Drift	16.1 nS/hr	$\leq 20.0$ nS/hr	PASS	1000

OVERALL TEST RESULT: PASS



Field Service Representative Signature:	Customer Signature:
<i>K. Hanthapong</i>	<i>Suman</i>
Date: 23/Apr/2024	Date: 23/Apr/2024

เอกสารไม่ควบคุม



## Information

<b>System Name</b>	Aquion RFIC
<b>Detector SN</b>	220360045
<b>Data Path</b>	ChromeleonLocal://Archemica/Service Contract/Validate 2024/1PM1PQ 23-04-24/Anion/IC OQ

## Peak Results

Sample Name	Injection Volume (μL)	Retention Time (min)	Area
Repeatability 01	25	0.265	2.825
Repeatability 02	25	0.265	2.822
Repeatability 03	25	0.265	2.831
Repeatability 04	25	0.265	2.835
Repeatability 05	25	0.265	2.834
Repeatability 06	25	0.265	2.836

## Repeatability

Test	Measured (% RSD)	OQ Limit (% RSD)	Result
Retention Time	0.0	≤ 5.0	PASS
Area	0.2	≤ 1.0	PASS

OVERALL TEST RESULT: PASS



Field Service Representative Signature:	Customer Signature:
<i>K. Gnanapavan</i>	<i>Srinan</i>
Date: 23/Apr/2024	Date: 23/Apr/2024

Information

System Name	Aquion RFIC
Detector SN	220360045
Data Path	ChromeleonLocal://Archemica/Service Contract/Validate 2024/1PM1PQ 23-04-24/Anion/IC OQ

Peak Results

Sample Name	Injection Volume (µL)	Retention Time (min)	Area
Reference Blank	25	0.265	0.053
High Standard	25	0.265	49.734
Carryover	25	0.265	0.051

Results


Test	Observed (%)	OQ Limit (%)	Result
AREA	0.00	≤ 0.10	PASS

OVERALL TEST RESULT: PASS



Field Service Representative Signature:	Customer Signature:
<i>K. Gammakorn</i>	<i>Suran</i>
Date: 23/Apr/2024	Date: 23/Apr/2024

เอกสารไม่ควบคุม

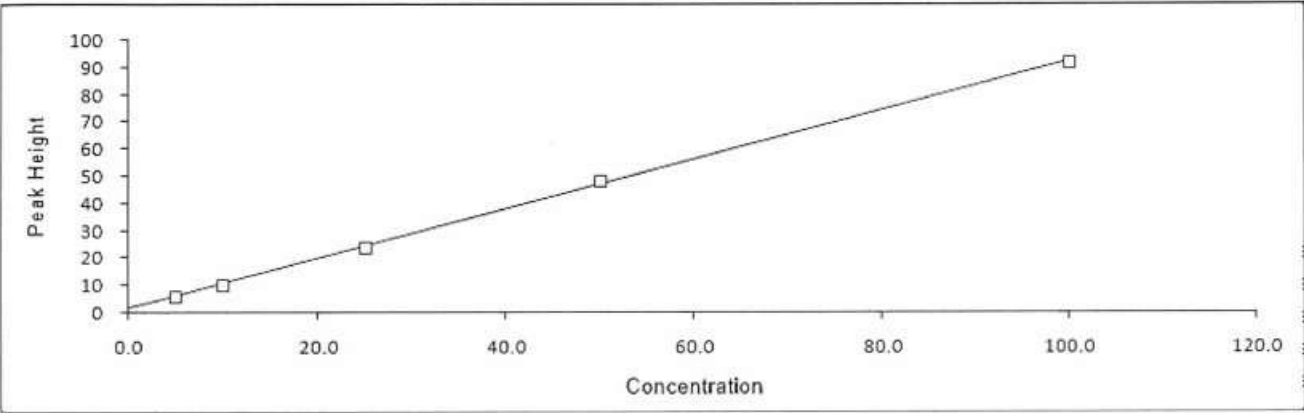

Information

System Name	Aquion RFIC
Detector SN	220360045
Data Path	ChromeleonLocal://Archemica/Service Contract/Validate 2024/1PM1PQ 23-04-24/Anion/IC OQ

Peak Results

Sample Name	Concentration	Peak Height	Calculated
Detector Linearity 01	5	5.872	4.82
Detector Linearity 02	10	10.299	9.68
Detector Linearity 03	25	23.794	24.52
Detector Linearity 04	50	48.473	51.65
Detector Linearity 05	100	91.855	99.34

Linearity

Test	Observed	OQ Limit	Result
$r^2$	0.999	$\geq 0.999$	PASS

OVERALL TEST RESULT: PASS





Field Service Representative Signature:	Customer Signature:
<i>K. R. R. R. R. R.</i>	<i>S. S. S. S. S.</i>
Date: 23/Apr/2024	Date: 23/Apr/2024

EG Current Test

Set Point (mM)	Expected (mA)	Reading (mA)	Deviation (mA)	OQ Limit (mA)	Result
1.00	1.6082	1.604	0.00	± 0.01	PASS
5.00	8.041	8.019	0.02	± 0.05	PASS
10.00	16.082	16.037	0.05	± 0.10	PASS
50.00	80.41	80.17	0.24	± 0.50	PASS
100.00	160.82	160.32	0.50	± 1.00	PASS

OVERALL TEST RESULT: PASS



Field Service Representative Signature:	Customer Signature:
	
Date: 23/Apr/2024	Date: 23/Apr/2024

เอกสารไม่ควบคุม





Column Compartment

Set Point (°C)	Reading (°C)	Deviation (°C)	OQ Limit (°C)	Result
30.0	30.5	0.5	± 2.0	PASS

OVERALL TEST RESULT: PASS



Field Service Representative Signature:	Customer Signature:
<i>K. Chandra Rao</i>	<i>Simam</i>
Date: 23/Apr/2024	Date: 23/Apr/2024

N/A

Remainder of Page Intentionally Blank



Field Service Representative Signature:	Customer Signature:
<i>K. Huanarong</i>	<i>Simon</i>
Date: <i>23/Apr/2024</i>	Date: <i>23/Apr/2024</i>

เอกสารไม่ควบคุม

These Operational Qualification Results should be reviewed by the Customer. If the qualification is accepted, both the Customer and the Service Representative should sign the Operational Qualification Results, below.

## OPERATIONAL QUALIFICATION RESULTS

Based upon the actual results obtained, this Operational Qualification **PASSED** the acceptance criteria described in the Operational Qualification in the Installation Checklist procedure.

### Service Representative

A Field Service Representative signature below confirms the completion of all aspects of the Operational Qualification and have concluded that the system has been successfully verified to be operating as required.

### Customer

A Customer signature below confirms the completion of all aspects of the Operational Qualification have been completed and that the system has been successfully verified to be operating as required.



Field Service Representative Signature:	Customer Signature:
<i>K. HANVACONG</i>	<i>Sumon</i>
Date: <i>23/Apr/2024</i>	Date: <i>23/Apr/2024</i>

# PinAAcle 900F Preventive Maintenance Report

Company Name:

Instrument Location:


Instrument Serial No.:

Date:

เอกสารไม่ควบคุม

## ***PinAAcle 900F Preventive Maintenance (PM)***

<b>Company Name:</b>			
<b>Address (Instrument Location):</b>			
<b>Serial Number:</b>		<b>PM Number:</b>	
<b>Customer Name (if applicable):</b>		<b>Telephone Number:</b>	
<b>Customer Support Engineer Name:</b>		<b>Service Order Number:</b>	
<b>Date PM Performed: (DD-MMM-YYYY)</b>		<b>Next PM Due Date: (DD-MMM-YYYY)</b>	
<b>Standard Labor Hours to Complete PM :</b>	<b>5 hours</b>		

Part Number	Release	Publication Date	
09370145 Rev.9	A	January 2018	

### **Scope**

The purpose of this PM is to ensure the continued functionality of the PinAAcle 900F by inspecting and replacing any worn or damaged parts. This service should only be performed by a trained representative of PerkinElmer.

The customer should save their method before the PM begins.

### **General Instructions:**

The customer must provide the engineer operational data to demonstrate recent instrument performance prior to starting the PM.

Always check with the customer before making any changes that may affect the customer's analysis or calibration, including a current back-up of system software and/or data files.

The completed document should be signed by an authorized PerkinElmer and customer representative and left with the customer.

Update the PM sticker and instrument logbook as required.

### **Copyright Information**

This document contains proprietary information that is protected by copyright. All rights are reserved.

No part of this publication may be reproduced in any form whatsoever or translated into any language without the prior, written permission of PerkinElmer, Inc.

**Copyright © 2013 PerkinElmer, Inc.**

### **Trademarks**

Registered names, trademarks, etc. used in this document, even when not specifically marked as such, are protected by law. PerkinElmer is a registered trademark of PerkinElmer, Inc. All other trademarks and registered trademarks not owned by PerkinElmer, Inc. or its subsidiaries that are depicted herein are the property of their respective owners. **Except as specifically set forth in its terms and conditions of sale, PerkinElmer makes no Warranty of any kind with regard to this document, including, but not limited to, the implied warranties of merchantability and fitness for a particular purpose.**

PerkinElmer shall not be liable for incidental or consequential damages in connection with the furnishing or use of this document.

## Component List

Component / Specific Model	Serial #	Configuration Notes

## Parts Lists

Parts Included with the PM		
Part Number (if applicable)	Description	Quantity
B0501696	Fan Filters	
N3160156	O-Ring Kits for Sampling Introduction ( Stainless Steels Nebulizer)	
N3160157	O-Ring Kits for Sampling Introduction ( Plastic Nebulizer)	
N9301714	Replacement Acetylene Filter Cartridge	
TH001022	Replacement Air Filter Cartridge	

Additional Reagents and Standards Required for PM				
Part Number (if applicable)	Description	Quality	Batch/Lot #	Expired Date (MM/YY)
N9300183	1000 mg/L Copper Standard	AR		

Additional Reagents and Standards Required for PM (Customer Support Solution)				
Part Number (if applicable)	Description	Quantity	Batch/Lot #	Expiration Date (MM/YY)
N/A	DI Water	250 ml.	AR	AR
N/A	0.5% HNO <sub>3</sub>	250 ml.	AR	AR



Additional Tools Required for PM			
Part Number (if applicable)	Description	Quantity	Serial #
N1013000	0.2A Neutral density filter	1	
N1013002	1.0A Neutral density filter	1	
03030997	System 2 EDL Driver	1	
N3050605	As System 2 EDL	1	
N3050121	Cu Lumina HCL	1	
N3050109	Ba Lumina HCL	1	
N3050139	K Lumina HCL	1	
N3050152	Ni Lumina HCL	1	

# Procedure Checklist

Use (✓) to check off those steps in the checklist that have been completed.

## 1. General:

- ☐ Review the instrument performance with the customer and document any recent problems.
- ☐ Inspect the customer log book and make any appropriate PM entries.
- ☐ Perform general inspection of system for cleanliness.

## 2. PC Instrument Software:

- ☐ Instrument Software user files/databases archived, packed, and/or deleted as needed.

## 3. Mechanical:

- ☐ Inspect and clean all fans and filters. Replace filters if necessary
- ☐ Inspect all gas lines for leaks and/or wear. Replace if needed.
- ☐ Clean exterior of the instrument.
- ☐ Inspect the burner head, burner chamber, and nebulizer. Clean if needed as stated in the Hardware Guide.
- ☐ Check burner head dimensions with the feeler gauge as stated in the Hardware Guide in the Maintenance chapter section on cleaning the burner head and checking sloth width. Replace if out of specification
- ☐ Check the condition of the end cap, burner head, and nebulizer O-rings. Replace if necessary.
- ☐ Check the drain system for signs of wear. Replace worn or damaged parts.
- ☐ Visually check for proper flame conditions when igniting the Air-C<sub>2</sub>H<sub>2</sub> and N<sub>2</sub>O-C<sub>2</sub>H<sub>2</sub> flames (if applicable).

## 4. Electrical:

- ☐ Inspect PC boards. Clean if necessary.
- ☐ Carefully check all internal and external cable connections.
- ☐ Check instrument firmware revisions upgrade to current levels (if necessary)
- ☐ Run Diagnostics Test within the Advanced function of the Spectrometer page. Check the results in the service log folder in the Spectrometer BM Log Viewer.

## 5. Optics:

- ☐ Inspect and clean the sample compartment windows, if needed.
- ☐ Inspect optics. Clean or replace if necessary,

## 6. Gasses:

- ☐ Verify that the Gasses supplied to the instrument are within the pressure and purity specifications found in the PinAAcle 900 Series Pre-installation Checklist SDB.
- ☐ Verify that the acetylene filter and air filter element is dry. Replace if necessary.

## 7. Flame Interlock Check:

Description: Check to ensure that all safety interlocks are closed.

Parameter	Specification	Test Results	Pass/Fail
Flame Sensor	Air/C <sub>2</sub> H <sub>2</sub> Flame correctly shuts down		
Drain Sensor	Air/C <sub>2</sub> H <sub>2</sub> Flame correctly shuts down		
Nebulizer Sensor	Air/C <sub>2</sub> H <sub>2</sub> Flame correctly shuts down		
C <sub>2</sub> H <sub>2</sub> Pressure Sensor	Air/C <sub>2</sub> H <sub>2</sub> Flame correctly shuts down		
Air Pressure Sensor	Air/C <sub>2</sub> H <sub>2</sub> Flame correctly shuts down		
Burner Head Sensor	Choosing Nitrous Oxide as the oxidant should trigger an interlock shuts down		

## 8. After PM Performance tests:

### 8.1 Detector Linearity with Barium

Description: Ensures that the detector is linear in the Visible Range.

Parameter	Specification	Certificate Value at 553.6 nm (Abs.)	Test Results	Pass/Fail
1.0 A ND Filter	± 5% from Cert.			
0.2 A ND Filter	± 5% from Cert.			

### 8.2 Baseline Noise at 1.0 Absorbance with Barium

Description: Ensures that a high absorbance will not produce excessive noise.

Parameter	Specification	Results	Pass/Fail
Standard Deviation	≤ 0.010		

### 8.3 AA Baseline Noise with Copper

Description: Check baseline noise.

Parameter	Specification	Results	Pass/Fail
Standard Deviation	≤ 0.001		

#### 8.4 D<sub>2</sub> Background Compensation with Copper

Description: Verifies the instruments ability to compensate for Background absorption.

Parameter	Specification	Results	Pass/Fail
Standard Deviation	≤ 0.010		

#### 8.5 AA-BG Baseline Noise with Copper

Description: Ensures that background correction does not produce excessive noise.

Parameter	Specification	Results	Pass/Fail
Standard Deviation	≤ 0.005		

#### 8.6 AA-BG Baseline Noise with Arsenic

Description: Ensures that background correction does not produce excessive noise at a low wavelength.

Parameter	Specification	Results	Pass/Fail
Standard Deviation	≤ 0.005		

#### 8.7 Flame Sensitivity

Description: Instrument Sensitivity checked against Copper standard.

Standard Copper Sensitivity	Specification	Results (Abs.)	Pass/Fail
5 mg/L Sensitivity SS Neb (if applicable)	> 0.250 Abs.		
2 mg/L Sensitivity HS Neb (if applicable)	> 0.250 Abs.		

#### 10. Review:

- ☐ Review with the customer PM work performed.
- ☐ Review with the customer routine maintenance procedures.
- ☐ Discuss recommended customer supplied materials to have on hand.
- ☐ Attach PM sticker.

## Additional Comments

### Additional Comments Regarding the PM

## Review

*The preventive maintenance checks and if applicable performance tests for PinAAcle 900F have been completed.*

*This PinAAcle 900F Passes ☐ Fails ☐ the preventive maintenance.*

### Review of Preventive Maintenance:

Authorized PerkinElmer Representative:

Chayanon R.

Date:

(DD-MMM-YYYY)

Authorized Customer Representative:

สุวิทย์ น้อย

Date:

(DD-MMM-YYYY)

## Agilent CrossLab Start Up Services

### Agilent 5100 5110 ICP-OES Preventive Maintenance



Agilent Preventive Maintenance provides factory recommended service for your analytical instruments to assure reliable operation and the accuracy of your results

Delivered by highly trained and certified service engineers using genuine Agilent parts and supplies, Agilent Preventive Maintenance provides what you need to reduce unplanned downtime and keep your systems operating at their peak performance.

This checklist is used as a guide for completing the preventive maintenance tasks. A signed copy of this checklist is provided for your records.



## Introduction

### Customer Information

- Customers should provide all necessary operating supplies upon request of the engineer.
- A customer representative should be available to the engineer while performing the preventive maintenance procedures. Customers are responsible for regular maintenance and are encouraged to observe the service representative.
- Any parts not included in the Parts Lists section of this document are not part of the recommended Preventive Maintenance service nor are they included in the price of this service.
- If a system requires the use of extra or special procedures and/or parts for the maintenance service, then these must be ordered separately and charged as a repair, which may incur additional costs.
- For customers using HF applications, the instrument should be returned to its standard sample introduction system.

## Important Customer Web Links

- To access **Agilent University**, visit <http://www.agilent.com/crosslab/university/> to learn about training options, which include online, classroom and onsite delivery. A training specialist can work directly with you to help determine your best options.
- To access the **Agilent Resource Center** web page, visit <https://www.agilent.com/en-us/agilentresources>. The following information topics are available:
  - Sample Prep and Containment
  - Chemical Standards
  - Analysis
  - Service and Support
  - Application Workflows
- The **Agilent Community** is an excellent place to get answers, collaborate with others about applications and Agilent products, and find in-depth documents and videos relevant to Agilent technologies. Visit <https://community.agilent.com/welcome>
- Videos about specific preparation requirements for your instrument can be found by searching the **Agilent YouTube** channel at <https://www.youtube.com/user/agilent>
- **Need to place a service call?** [Flexible Repair Options | Agilent](#)

## Service Engineer's Responsibilities

- Contact the customer and ensure that all necessary supplies are available before the preventive maintenance visit.
- Only select those pages that relate to the system or module being serviced.
- Complete empty fields with the relevant information.
- Complete the relevant checkboxes in the checklist using either a "X" or tick mark "✓".
- Check **"Service not applicable"** check boxes to indicate services/tasks not delivered, as appropriate.
- Complete the Preventive Maintenance services in the most logical order relevant to the individual system service in the order of the tasks listed.
- Complete the **Service Review** section together with the customer.
- Complete the fields for page numbers at the foot of each selected page
- Add relevant page numbers to selected pages and complete the total number of pages field in the Service Completion section
- **Ask the customer to sign the Service Verification section including the customer's and your signature.**

## Instrument Maintenance

### System Information

- ☐ Check this box if an instrument configuration report is attached instead of completing the table.

Instrument System Name and ID	5110 VDV ICP-OES
Instrument System Site and Location	United Analyst and Engineering Consultant

List System Component Product Numbers	List the Serial Numbers of each Component
1. G 8015A	MY 18030001
2.	
3.	
4.	
5.	
6.	
7.	
8.	
9.	

ICP-OES Configuration Table	Circle the type or write in the type if other
Nebulizer Type	SeaSpray (OneNeb) Conikal   Other
Spray Chamber	Cyclonic Single Pass (Cyclonic Double Pass) Other
Torch	Radial (Dual View) Other
Torch Type	One Piece (Semi Demountable) Fully Demountable   Other
Injector Diameter	2.4mm (1.8mm) 1.4mm   0.8mm   Other
Injector Material	(Quartz) Ceramic   Other

## Preparation

- ☒ Discuss any specific issues with the customer before starting.
- ☒ Review the instrument logbook for recorded problems and comments.
- ☒ Save instrument control settings before starting the procedure.
- ☒ Perform a general inspection of the system for cleanliness.
- ☒ Check for proper installation of parts, assemblies, sensors etc.
- ☒ Check system for required installation of components and implementation of Service Notes
- ☒ Check for required firmware/software updates and verify with customers if they would like them installed.
- ☐ For HF application systems, if standard sample introduction system was not installed, ask the customer to install it. ๙๑๖
- ☒ Ask the customer to remove any samples from the ICP-OES sample introduction area, auto sampler or around the ICP-OES.



## Preventive Maintenance Procedures

### Record Pre-PM instrument performance

- ☒ Run Instrument Performance test.
- ☒ Record results in Instrument Performance Test Results Table – Pre-PM.

### Clean and inspect ICP-OES system

- ☒ Look for any obvious external damage or problems.
- ☒ Inspect water cooling hoses, gas lines and power cord for excessive wear or damage.
- ☒ Perform a general internal inspection of the system for excessive dust accumulation, clean if necessary.
- ☒ Inspect sample introduction components and record any required maintenance in the Service Engineer Comments and notify the customer as the required actions required.
- ☒ Record the instrument operating conditions in the ICP-OES Status Results Table.
- ☒ Replace the polychromator purge filter.
- ☒ Replace the radial pre-optics window
- ☒ Replace the axial pre-optics window for SVDV and VDV instruments.
- ☒ Check exhaust flow for the correct positive extraction at the exhaust duct to insure they meet minimum specifications.
- ☒ Replace air inlet dust filter.
- ☐ Replace high capacity air inlet dust filter element if installed. N/A
- ☒ Remove and clean instrument water inlet filter.

### Agilent Water Recirculator

- ☐ **Service not applicable**
- ☒ Drain cooling fluid and remove any particles from the chiller reservoir
- ☒ Remove, clean and reinstall water inlet metal mesh filter if present.
- ☒ Re fill with Agilent Cool Clear cooling fluid.
- ☒ Clean the cooling system Air filter and the condenser.

### SPS 3 Auto Sampler

- ☒ **Service not applicable**
- ☐ Power cycle the autosampler and verify successful initialization.
- ☐ Inspect X and Z axis belts for wear. Replace is necessary.
- ☐ Clean X and Z axis slide shafts.
- ☐ Using customer's racks and the Agilent software move the sample probe to the 4 outermost corners and rinse port, ensure that the probe is approximately centered in the vial.

### SPS 4 Auto sampler

- ☒ **Service not applicable**
- ☐ Clean the spill tray, rack location mat, end frames and chassis with a damp soft cloth and diluted mild detergent.
- ☐ Clean the auto sampler cover panels, if cover kit is installed, with domestic window cleaner.
- ☐ Check the X-axis and Z-axis drive belts for cracks, splits, damaged teeth, excessive fraying, color changes or degradation from fumes.
- ☐ Check the X-axis, Theta-axis and Z-axis FFC cables for cracks, incorrect positioning, damaged edges or damaged connectors.
- ☐ Pump Tubing Replacement. Replace peristaltic pump tubing. Replace all tubing that goes from the rinse station to the pump and from the pump to the waste/rinse bottles
- ☐ Test using customer's tray and move the sample probe to the sample vial 1, wash vial and rinse port and ensure that the probe is centered in the vial. If not use calibration wizard and calibrate the position.

### AVS 4, 6, 7 Advanced Valve System

- ☒ **Service not applicable**
- ☐ Replace valve rotor seal
- ☐ Check fittings for signs of leaks
- ☐ Check tubing including autosampler tubing for kinks or excessive wear
- ☐ Check high flow pump for signs of leaks



## ICP-OES adjustment

- ☒ Check position of Zn peak, adjust if required.
- ☒ Check Argon Ratio, adjust to specified value if required.
- ☒ Perform Detector Calibration.
- ☒ Perform Instrument Calibration.

## Record Post-PM instrument performance

- ☒ Run Instrument Performance test.
- ☒ Record results in Instrument Performance Test Results Table - Post PM.
- ☒ For systems using ICP Expert version 7.3 and above, run the following Instrument tests
  - ☒ Subsystem Communications Test
  - ☒ Air Flow
  - ☒ Water Flow
  - ☒ Gas Flows
  - ☒ RF Generator
  - ☒ Camera Test
  - ☒ Optics Test
  - ☒ Nebulizer Test
- ☒ Record the result in the Instrument Test Results Table

## Restore Instrument

- ☐ For HF applications, ask the customer to reinstall their sample introduction system. N/A
- ☒ Leave system in an idle state: on and purging.
- ☒ Guidance: If the PM service is performed prior to a qualification service, then use the qualification procedure as a guide for final instrument set up and checkout.

## Service Review

- ☒ Attach available reports/printouts of all tests to this documentation.
- ☒ Record the Preventive Maintenance service activity in the customer's records/logbook.
- ☒ Record the PM event in the Smart Alerts logbook, if applicable.
- ☒ Update/reset instrument maintenance counters as appropriate.
- ☒ Affix the PM sticker to the system or instrument logbook based on the customer's request.
- ☒ Complete the Service Engineer Comments section if there are additional comments.
- ☒ Review this service, parts replaced, and test results obtained with the customer.
- ☒ If the instrument firmware was updated, record the details of the change in the Service Engineer's Comments box. Systems in a compliant environment may need additional documentation.
- ☒ **Complete the Signature Page with both Service Engineer and Customer signatures.**

## Test Results

### Instrument Performance Test Results Table

Note: These measurements do not form part of any specification and are for reference only.

	Pre PM Sensitivity Check		Post PM Sensitivity Check	
	Radial	Axial *	Radial	Axial*
Zn 213.857 nm SRBR	1500.8	2217.4	4124.8	6965.9
Mn 257.610 nm SRBR	3915.0	7492.2	13017.8	31121.6
Al 396.152 nm SBR	7.7	10.7	9.7	21.1
K 766.491 nm SBR	5.7	28.1	4.8	45.3

\* Axial result is not applicable for G8016AA, G8012AA Radial View instruments.

### Instrument Test Results Table

Note: The Instrument Test results are for systems using ICP Expert version 7.3 and above only.

Instrument Test	Result
Subsystem Communications Test	Pass
Air Flow	Pass
Water Flow	Pass
Gas Flows	Pass
RF Generator	Pass
Camera Test	Pass
Optics Test	Pass
Nebulizer test	Pass

## ICP-OES Status Results Table

Note: These measurements do not form part of any specification and are for reference only.

Measurement	Standby Mode		Plasma On	
Mains Voltage	231.411	VAC	226.871	VAC
Mains Current	0.081	A	0.105	A
Instrument Temperature	22.1	°C	23.5	°C
RF Air Flow (sensor speed)	14.0	Hz	19.0	Hz
Plasma Exhaust Temperature	No measurement		63.8	°C
Water Flow Oscillator	No measurement		1.34	L/min
Water Flow Detector	0.86	L/min	0.81	L/min
Water Inlet Temperature	19.7	°C	19.7	°C
Polychromator Temperature	35.0	°C	35.0	°C
CCD Temperature	-40.1	°C	-39.8	°C
Thermal Stabilizer	35.0	°C	35.0	°C
Argon Supply Pressure	648.92	kPa	591.55	kPa
Purge Gas Supply Pressure*1	646.66	kPa	612.41	kPa
Option Gas Supply Pressure*1	-	kPa	-	kPa
Nebulizer Flow	No measurement		0.70	L/min
Nebulizer Back Pressure	No measurement		158.43	kPa
Plasma Gas Flow	No measurement		11.91	L/min
Auxiliary Gas Flow	No measurement		1.00	L/min
RF Power	No measurement		1204.7	W
RF Supply Current	No measurement		7.858	A
RF Supply Voltage	No measurement		204.417	V

\*1 If option installed



## Consumed PM Parts

Part Description	Part Number	Product or Model# where used	Quantity consumed
Axial Pre-Optic Window	G8010-68014	G8010A, G8011A, G8014A/G8015A	1
Radial Pre-Optic Window	G8010-68015	All	1
Agilent Cool Clear Coolant Fluid	5799-0037	Agilent Water Recirculator	-
Purge Gas Filter	G8010-60136	All	1
Air inlet filter	G8000-68002	All	1
High Capacity Air Filter	G8010-60189	Optional	-
Rotor seal for 6-7 port valve for AVS6/7	G8494-60002	G8494A/G8495	-
Rotor seal for 4 port valve for AVS4	G8493-60002	G8493A	-
Rinse solution to rinse station 2.5mm id x 1m	G8410-80123	SPS 4	-
Barb connector 2.5mm-1.5mm ID	G8410-80124	SPS 4	-
PVC waste tubing, 8mm od x 5mm id, 2m	G8410-80122	SPS 4	-
<b>Additional Parts may be required from engineer's stock:</b>			
X axis drive belt	5410047500	SPS 3	-
Z axis drive belt	5410047400	SPS 3	-
Peristaltic pump tubing, PVC SolvaFlex, 3 bridged,	3710049000	SPS 4	-

## Consumed Parts Reference (Purchased by customer, not included as part of PM)

☒ Section Not Applicable.

Part Description	Part Number	Product or Model# where used	Quantity consumed

## Signature Page

### Service Engineer Comments (optional)

If there are any specific points you wish to note as part of performing the installation or other items of interest for the customer, please write in this box.

## Service Verification

Service Request Number:

6007197100

Service Engineer Name:

Kanyakorn S.

Service Engineer Signature:

Kanyakorn S.

Total number of pages in this document:

14

Date Service Completed:

04 Nov 2024

Customer Name:

Aphorn Onkong

Customer Signature:

Aphorn Onkong

**Report Summary**

Instrument Model	Agilent 5100/5110 VDV ICP-OES
Instrument ID	G8011A/G8015A
Instrument Serial Number	MY18030001
Software Version	7.3.1.9507
Firmware Version	3442
Tested By	Pre Test_PM_Kanyakorn S.
Test Completed On	11/4/2024 9:19:10 AM

**Result Summary**

Subsystem Communications Test	Skipped
Air Flow Test	Skipped
Water Flow Test	Skipped
Gas Flows Test	Skipped
RF Generator Test	Skipped
Camera Test	Skipped
Optics Test	Skipped
Advanced Valve System Test	Skipped
Resolution Test	Pass
Sensitivity Test	Fail
Precision Test	Pass



**Resolution Test****Pass**

Element Wavelength	Specification	Width
N (174.213 nm)	≤ 9.40	6.98
As (188.980 nm)	≤ 8.20	6.17
C (193.027 nm)	≤ 11.50	8.30
Mo (202.032 nm)	≤ 8.20	6.38
Cr (206.158 nm)	≤ 13.40	8.98
Zn (213.857 nm)	≤ 8.70	6.60
Pb (220.353 nm)	≤ 9.50	7.09
Co (228.615 nm)	≤ 17.20	11.67
Ba (230.424 nm)	≤ 9.40	7.20
Mn (257.610 nm)	≤ 13.30	9.43
Mn (260.568 nm)	≤ 20.30	14.11
Cr (267.716 nm)	≤ 11.00	8.04
Cu (324.754 nm)	≤ 25.00	18.97
Cu (327.395 nm)	≤ 14.20	11.23
Sr (338.071 nm)	≤ 33.50	24.30
Ba (455.403 nm)	≤ 44.00	33.47
Sr (460.733 nm)	≤ 36.00	17.23
Ba (493.408 nm)	≤ 36.00	25.37
Ba (614.171 nm)	≤ 42.00	25.54
Ar (675.283 nm)	≤ 74.00	56.51
K (766.491 nm)	≤ 80.00	65.86

**Sensitivity Test****Fail****Radial**

Element Wavelength	Specification	Method	Ratio	Standard	Blank
As (188.980 nm)	≥ 46.0	SRBR	104.1	793.0	50.8
Se (196.026 nm)	≥ 41.0	SRBR	87.6	862.0	79.7
Zn (213.857 nm)	≥ 1421.0	SRBR	1500.8	41823.3	749.0
Pb (220.353 nm)	≥ 46.0	SRBR	170.7	2432.0	174.9
Mn (257.610 nm)	≥ 3518.0	SRBR	3915.0	264700.2	4420.0
Al (396.152 nm)	≥ 3.4	SBR	7.7	48454.6	5563.2
Ba (493.408 nm)	≥ 34.0	SBR	45.9	1966719.7	41903.8
K (766.491 nm)	≥ 1.8	SBR	5.7	99036.2	14687.7

**Axial**

Element Wavelength	Specification	Method	Ratio	Standard	Blank
As (188.980 nm)	≥ 208.0	SRBR	126.5	1498.8	119.0
Se (196.026 nm)	≥ 159.0	SRBR	112.0	1773.6	197.8
Zn (206.200 nm)	≥ 234.0	SRBR	466.0	6784.2	199.7
Zn (213.857 nm)	≥ 1743.0	SRBR	2217.4	95597.6	1789.7
Cd (214.439 nm)	≥ 4227.0	SRBR	1919.3	68724.6	1236.4
Pb (220.353 nm)	≥ 320.0	SRBR	332.6	7929.5	499.0
Mn (257.610 nm)	≥ 10625.0	SRBR	7492.2	991238.3	16911.7
Cr (267.716 nm)	≥ 1048.0	SRBR	2254.6	129706.6	3150.9
Cu (324.754 nm)	≥ 19.0	SBR	26.9	290746.3	10407.5
Al (396.152 nm)	≥ 6.0	SBR	10.7	211329.2	18005.0
Ba (493.408 nm)	≥ 60.0	SBR	49.3	6956460.4	138336.9
K (766.491 nm)	≥ 24.0	SBR	28.1	1395190.2	47996.2

## Precision Test

Pass

## Radial

Element Wavelength	Specification	Measured Value % RSD
As (188.980 nm)	$\leq 2.60$	0.73
Se (196.026 nm)	$\leq 2.60$	0.95
Zn (213.857 nm)	$\leq 1.50$	0.31
Pb (220.353 nm)	$\leq 2.60$	0.73
Mn (257.610 nm)	$\leq 1.50$	0.39
Al (396.152 nm)	$\leq 1.50$	0.39
Ba (493.408 nm)	$\leq 1.50$	0.87
K (766.491 nm)	$\leq 1.50$	0.32

## Axial

Element Wavelength	Specification	Measured Value % RSD
As (188.980 nm)	$\leq 1.50$	1.21
Se (196.026 nm)	$\leq 1.50$	0.84
Zn (206.200 nm)	$\leq 1.50$	0.56
Zn (213.857 nm)	$\leq 1.50$	0.96
Cd (214.439 nm)	$\leq 1.50$	0.26
Pb (220.353 nm)	$\leq 1.50$	0.51
Mn (257.610 nm)	$\leq 1.50$	0.97
Cr (267.716 nm)	$\leq 1.50$	0.22
Cu (324.754 nm)	$\leq 1.50$	0.24
Al (396.152 nm)	$\leq 1.50$	0.33
Ba (493.408 nm)	$\leq 1.50$	0.40
K (766.491 nm)	$\leq 1.50$	0.65

### Report Summary

Instrument Model	Agilent 5100/5110 VDV ICP-OES
Instrument ID	G8011A/G8015A
Instrument Serial Number	MY18030001
Software Version	7.3.1.9507
Platform	3442
Tested By	Post Test_PM_Kanyakorn S.
Test Completed On	11/4/2024 11:07:24 AM

### Result Summary

Subsystem Communications Test	Pass
Air Flow Test	Skipped
Water Flow Test	Skipped
Gas Flows Test	Skipped
RF Generator Test	Skipped
Camera Test	Skipped
Optics Test	Pass
Advanced Valve System Test	Skipped
Resolution Test	Pass
Sensitivity Test	Fail
Precision Test	Pass
Subsystem Communications Test	Pass

### Optics Test

	Radial	Axial
Intensity	3184054	3177175
Wavelength	737.212	737.212

Resolution Test		Pass
Element Wavelength	Specification	Width
N (174.213 nm)	≤ 9.40	6.97
As (188.980 nm)	≤ 8.20	6.14
C (193.027 nm)	≤ 11.50	8.33
Mo (202.032 nm)	≤ 8.20	6.33
Cr (206.133 nm)	≤ 13.40	9.06
Zn (213.637 nm)	≤ 8.70	6.70
Pb (220.353 nm)	≤ 9.50	7.03
Co (228.615 nm)	≤ 17.20	11.72
Ba (230.424 nm)	≤ 9.40	7.32
Mn (257.610 nm)	≤ 13.30	9.44
Mn (260.568 nm)	≤ 20.30	14.21
Cr (267.716 nm)	≤ 11.00	7.94
Cu (324.754 nm)	≤ 25.00	18.99
Cu (327.395 nm)	≤ 14.20	11.27
Sr (338.071 nm)	≤ 33.50	24.40
Ba (455.403 nm)	≤ 44.00	33.50
Sr (460.733 nm)	≤ 36.00	17.31
Ba (493.408 nm)	≤ 36.00	25.44
Ba (614.171 nm)	≤ 42.00	25.16
Ar (675.283 nm)	≤ 74.00	56.15
K (766.491 nm)	≤ 80.00	65.56

## Sensitivity Test

Fail

## Radial

Element Wavelength	Specification	Method	Ratio	Standard	Blank
As (188.980 nm)	≥ 46.0	SRBR	130.6	977.1	50.4
Se (196.026 nm)	≥ 41.0	SRBR	106.0	958.7	70.2
Zn (213.857 nm)	≥ 1421.0	SRBR	4124.8	44037.7	113.4
Pb (220.353 nm)	≥ 46.0	SRBR	207.2	2554.7	136.2
Mn (257.610 nm)	≥ 3518.0	SRBR	13017.8	271846.6	434.7
Al (396.152 nm)	≥ 3.4	SBR	9.7	50615.5	4717.0
Ba (493.408 nm)	≥ 34.0	SBR	133.7	2069203.0	15359.3
K (766.491 nm)	≥ 1.8	SBR	4.8	100199.5	17235.5

## Axial

Element Wavelength	Specification	Method	Ratio	Standard	Blank
As (188.980 nm)	≥ 208.0	SRBR	174.9	1566.7	73.0
Se (196.026 nm)	≥ 159.0	SRBR	167.0	1863.4	110.2
Zn (206.200 nm)	≥ 234.0	SRBR	740.9	6836.0	83.1
Zn (213.857 nm)	≥ 1743.0	SRBR	6965.9	101568.1	211.7
Cd (214.439 nm)	≥ 4227.0	SRBR	5781.0	72852.9	158.1
Pb (220.353 nm)	≥ 320.0	SRBR	501.0	8464.3	267.7
Mn (257.610 nm)	≥ 10625.0	SRBR	31121.6	1006637.8	1044.0
Cr (267.716 nm)	≥ 1048.0	SRBR	4424.8	132202.9	880.8
Cu (324.754 nm)	≥ 19.0	SBR	68.7	302907.8	4345.6
Al (396.152 nm)	≥ 6.0	SBR	21.1	218771.0	9892.3
Ba (493.408 nm)	≥ 60.0	SBR	250.6	7137380.9	28367.3
K (766.491 nm)	≥ 24.0	SBR	45.3	1435050.6	31025.0

## Precision Test

Pass

## Radial

Element Wavelength	Specification	Measured Value % RSD
As (188.980 nm)	$\leq 2.60$	0.81
Se (196.026 nm)	$\leq 2.60$	0.98
Zn (213.857 nm)	$\leq 1.50$	0.22
Pb (220.353 nm)	$\leq 2.60$	0.37
Mn (257.610 nm)	$\leq 1.50$	0.27
Al (396.152 nm)	$\leq 1.50$	0.25
Ba (493.408 nm)	$\leq 1.50$	0.53
K (766.491 nm)	$\leq 1.50$	0.15

## Axial

Element Wavelength	Specification	Measured Value % RSD
As (188.980 nm)	$\leq 1.50$	0.81
Se (196.026 nm)	$\leq 1.50$	0.65
Zn (206.200 nm)	$\leq 1.50$	0.79
Zn (213.857 nm)	$\leq 1.50$	0.81
Cd (214.439 nm)	$\leq 1.50$	0.35
Pb (220.353 nm)	$\leq 1.50$	0.33
Mn (257.610 nm)	$\leq 1.50$	1.02
Cr (267.716 nm)	$\leq 1.50$	0.32
Cu (324.754 nm)	$\leq 1.50$	0.51
Al (396.152 nm)	$\leq 1.50$	0.37
Ba (493.408 nm)	$\leq 1.50$	0.68
K (766.491 nm)	$\leq 1.50$	0.74



**Report Summary**

Instrument Model	Agilent 5100/5110 VDV ICP-OES
Instrument ID	G8011A/G8015A
Instrument Serial Number	MY18030001
Software Version	7.3.1.9507
Firmware Version	3442
Tested By	Post Test_PM_Kanyakorn S.
Test Completed On	11/4/2024 11:30:15 AM

**Result Summary**

Subsystem Communications Test	Pass
Air Flow Test	Pass
Water Flow Test	Pass
Gas Flows Test	Pass
RF Generator Test	Pass
Camera Test	Pass
Optics Test	Skipped
Advanced Valve System Test	Skipped
Resolution Test	Skipped
Sensitivity Test	Skipped
Precision Test	Skipped

Subsystem Communications Test	Pass
-------------------------------	------

Air Flow Test	Pass
---------------	------

30% Air Flow (relative speed)	75% Air Flow (relative speed)
15.00	19.00

Water Flow Test	Pass
-----------------	------

RF Water Flow(L/min)	Camera Water Flow (L/min)	Water Inlet Temperature (°C)
1.30	0.81	20.55

**Gas Flows Test****Pass**

Nebulizer Target Flow	Actual Flow	Back Pressure	Auxiliary Target Flow	Actual Flow	Back Pressure
0.70	0.70	154.65	2.00	2.00	110.92
Makeup Target Flow	Actual Flow	Back Pressure	Plasma Target Flow	Actual Flow	Back Pressure
2.00	2.00	115.38	18.00	17.97	21.48

**RF Generator Test****Pass**

RF Power Supply Test	Passed
RF Power Supply (V)	128.554
RF Oscillator Test	Passed
RF Oscillator Frequency (MHz)	25.834
Work Coil Current (A)	44.660
RF Power Supply Current (A)	1.999

**Camera Test****Pass**

	Integration Time (ms)	Standard Deviation	Status
Electronic Offset Test	1000	5.228	Passed
Dark Current Test	6000	1.168	Passed
Array Test	5	0.024	Passed
Linearity Test		0.118	Passed

### Report Summary

Instrument Model	Agilent 5100/5110 VDV ICP-OES
Instrument ID	G8011A/G8015A
Instrument Serial Number	MY18030001
Software Version	7.3.1.9507
Firmware Version	3442
Tested By	change mirror
Test Completed On	11/6/2024 10:35:26 AM

### Result Summary

Subsystem Communications Test	Skipped
Air Flow Test	Skipped
Water Flow Test	Skipped
Gas Flows Test	Skipped
RF Generator Test	Skipped
Camera Test	Skipped
Optics Test	Skipped
Advanced Valve System Test	Skipped
Resolution Test	Pass
Sensitivity Test	Pass
Precision Test	Pass

**Resolution Test****Pass**

Element Wavelength	Specification	Width
N (174.213 nm)	$\leq 9.40$	6.79
As (188.980 nm)	$\leq 8.20$	5.80
C (193.027 nm)	$\leq 11.50$	8.15
Mo (202.032 nm)	$\leq 8.20$	5.90
Cr (206.158 nm)	$\leq 13.40$	8.85
Zn (213.857 nm)	$\leq 8.70$	6.77
Pb (220.353 nm)	$\leq 9.50$	6.61
Co (228.615 nm)	$\leq 17.20$	11.79
Ba (230.424 nm)	$\leq 9.40$	7.25
Mn (257.610 nm)	$\leq 13.30$	9.47
Mn (260.568 nm)	$\leq 20.30$	14.50
Cr (267.716 nm)	$\leq 11.00$	7.91
Cu (324.754 nm)	$\leq 25.00$	18.72
Cu (327.395 nm)	$\leq 14.20$	11.09
Sr (338.071 nm)	$\leq 33.50$	25.39
Ba (455.403 nm)	$\leq 44.00$	33.09
Sr (460.733 nm)	$\leq 36.00$	18.54
Ba (493.408 nm)	$\leq 36.00$	25.74
Ba (614.171 nm)	$\leq 42.00$	25.23
Ar (675.283 nm)	$\leq 74.00$	58.92
K (766.491 nm)	$\leq 80.00$	63.16

**Sensitivity Test****Pass****Radial**

Element Wavelength	Specification	Method	Ratio	Standard	Blank
As (188.980 nm)	≥ 46.0	SRBR	110.5	868.9	54.3
Se (196.026 nm)	≥ 41.0	SRBR	88.3	934.7	91.3
Zn (213.857 nm)	≥ 1421.0	SRBR	3535.4	44017.7	153.9
Pb (220.353 nm)	≥ 46.0	SRBR	184.5	2492.3	159.8
Mn (257.610 nm)	≥ 3518.0	SRBR	11099.6	249595.3	503.6
Al (396.152 nm)	≥ 3.4	SBR	8.7	50274.4	5172.0
Ba (493.408 nm)	≥ 34.0	SBR	124.5	1903164.1	15166.0
K (766.491 nm)	≥ 1.8	SBR	6.9	110041.4	13991.2

**Axial**

Element Wavelength	Specification	Method	Ratio	Standard	Blank
As (188.980 nm)	≥ 208.0	SRBR	253.3	3744.3	196.3
Se (196.026 nm)	≥ 159.0	SRBR	206.7	4199.7	347.2
Zn (206.200 nm)	≥ 234.0	SRBR	923.0	12282.3	172.1
Zn (213.857 nm)	≥ 1743.0	SRBR	6398.3	157551.5	601.7
Cd (214.439 nm)	≥ 4227.0	SRBR	5069.2	99873.7	385.2
Pb (220.353 nm)	≥ 320.0	SRBR	389.0	10641.1	658.6
Mn (257.610 nm)	≥ 10625.0	SRBR	21190.4	985528.7	2153.6
Cr (267.716 nm)	≥ 1048.0	SRBR	3054.1	131797.6	1811.5
Cu (324.754 nm)	≥ 19.0	SBR	36.3	301401.4	8082.9
Al (396.152 nm)	≥ 6.0	SBR	10.8	228359.5	19280.5
Ba (493.408 nm)	≥ 60.0	SBR	106.5	6460421.5	60122.8
K (766.491 nm)	≥ 24.0	SBR	30.2	1639840.6	52562.1

**Precision Test****Pass****Radial**

Element Wavelength	Specification	Measured Value % RSD
As (188.980 nm)	$\leq 2.60$	1.56
Se (196.026 nm)	$\leq 2.60$	1.16
Zn (213.857 nm)	$\leq 1.50$	0.50
Pb (220.353 nm)	$\leq 2.60$	0.74
Mn (257.610 nm)	$\leq 1.50$	0.63
Al (396.152 nm)	$\leq 1.50$	0.54
Ba (493.408 nm)	$\leq 1.50$	0.78
K (766.491 nm)	$\leq 1.50$	0.44

**Axial**

Element Wavelength	Specification	Measured Value % RSD
As (188.980 nm)	$\leq 1.50$	0.82
Se (196.026 nm)	$\leq 1.50$	0.82
Zn (206.200 nm)	$\leq 1.50$	0.35
Zn (213.857 nm)	$\leq 1.50$	0.34
Cd (214.439 nm)	$\leq 1.50$	0.44
Pb (220.353 nm)	$\leq 1.50$	0.48
Mn (257.610 nm)	$\leq 1.50$	0.83
Cr (267.716 nm)	$\leq 1.50$	0.53
Cu (324.754 nm)	$\leq 1.50$	0.69
Al (396.152 nm)	$\leq 1.50$	0.56
Ba (493.408 nm)	$\leq 1.50$	1.29
K (766.491 nm)	$\leq 1.50$	0.74


## Calibration Certificate

**Certificate No.:** 2401718-001-01  
**Client name:** UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.  
**Address:** 3 Soi Udomsuk 41, Sukhumvit Road,  
Bangchack, Prakhonong, Bangkok 10260

Page 1 of 5

**Equipment:** pH Meter  
**Manufacturer:** METTLER TOLEDO  
**Model:** SevenEasy pH  
**Serial No.:** 1231155210  
**ID No.:** UAE.WAT.010/2553  
**Order No.:** 2401718  
**Operation No.:** 2401718-001  
**Date of Receipt:** 27 February 2024  
**Date of Calibration:** 11 March 2024

**Calibrated by** Mr.Manas Somsak  
Specialist

**Approved by**   
( Mr.Pheraphat Tuanjit )

Manager, Division of Calibration Laboratory

**Date of Issue:** 12 March 2024

Responsible for the Technical Management Team

The uncertainties are for a confidence probability of approximately 95%.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the National Food Institute.

F-CS-009 Revision: 01 Date: 20-04-65





## Calibration Report

**Certificate No.:** 2401718-001-01

**Equipment:** pH Meter **Resolution:** 0.01 pH ; 1 mV  
**Manufacturer:** METTLER TOLEDO **Model:** SevenEasy pH  
**Serial No.:** 1231155210 **Type:** Bench top  
**ID No.:** UAE.WAT.010/2553

**Date of Calibration:** 11 March 2024

Page 2 of 5

**Location:** Chemical Calibration Laboratory, National Food Institute

**Environment Condition:** **Ambient Temperature:** ( 23.4 ± 1.5 ) °C **Relative Humidity:** ( 51 ± 3 ) %

**Condition of Equipment:** Good Condition

### Condition of this Results of Calibration

1. Calibration Method W-CC-002 : In house method based on direct measurement by using standard voltage calibrator and certified reference material (CRM)

### 2. Reference Standards / Certified Reference Material

Instruments	Serial / ID No.	Manufacturer	Certificate No.	Due Date
2.1 DC Voltage Calibrator	2709007	Fluke	23E2003	14 June 2024
2.2 Digital Thermometer	2709007	Fluke	CC 660570-01	30 October 2024
2.3 Thermo-Hygro Meter	NFI.BTH 014/23	testo	CC 660353-01	3 April 2024
Certified Reference Material	Lot. No.	Manufacturer	Ref N	Expire Date
2.4 pH buffer 4.008 (Primary pH buffer Solution)	888842	CPAchem	PH216.L5	13 April 2025
2.5 pH buffer 6.865 (Primary pH buffer Solution)	888843	CPAchem	PH217.L5	13 April 2025
2.6 pH buffer 10.01 (Primary pH buffer Solution)	888844	CPAchem	PH220.L5	13 April 2024
2.7 pH buffer 7.00 (Standard pH buffer Solution)	C03109	HACH LANGE GmbH	S11M004	16 October 2025

### 3. This certification is traceable to The International System of Unit (SI Unit)

3.1 Instruments No.2.1	through	NSC-TISI-TIS 17025 Laboratory Accreditation of Calibration No.0008
3.2 Instruments No.2.2 and 2.3	through	NSC-TISI-TIS 17025 Laboratory Accreditation of Calibration No.0061
3.3 Certified Reference Material No.2.4 to 2.6	traceable to	Primary measurement method- Harned cell using calibrated thermometer, barometer, and nanovoltmeter. The Standard Solution preparation and certified by CPAchem Ltd is accredited to ISO 17034 and ISO/IEC 17025
3.4 Certified Reference Material No.2.7	traceable to	PTB Certificate Nr. PTB-PHOA-563/30504/23 and Certificate Nr. PTB-PHOB-555/30620/22 (PTB: Physikalisch-Technische Bundesanstalt, Braunschweig, Germany)

4. This certificate was certified only for the instrument we calibrated.

5. This result of calibration was found accurate as shown on date and place of calibration only.



F-CS-012 Revision: 01 Date: 20-04-65

## Calibration Report

**Certificate No.:** 2401718-001-01

**Equipment:** pH Meter **Resolution:** 0.01 pH ; 1 mV

**Manufacturer:** METTLER TOLEDO **Model:** SevenEasy pH

**Serial No.:** 1231155210 **Type:** Bench top

**ID No.:** UAE.WAT.010/2553

**Date of Calibration:** 11 March 2024

Page 3 of 5

### Calibration Results:

#### 1. Calibration of pH Meter ( Manual Temperature Compensation at 25 °C )

(offset value before adjust: -0.4 mV)

Nominal pH	DC Voltage Standard ( mV )	Average Indicator Reading		Uncertainty ( ±mV )	Coverage Factor ( k )
		mV	pH		
0	414.121	414	0.00	0.58	2.00
2	295.814	296	2.00	0.58	2.00
4	177.464	178	4.00	0.58	2.00
6	59.160	59	6.00	0.58	2.00
7	0.001	0	7.00	0.58	2.00
8	-59.159	-59	8.00	0.58	2.00
10	-177.461	-177	10.00	0.58	2.00
12	-295.811	-296	12.00	0.58	2.00
14	-414.118	-414	14.00	0.58	2.00

#### 2. Calibration of pH Meter with Electrode ( Manual Temperature Compensation at 25 °C )

**Equipment:** pH Electrode **Type:** Combined Electrode

**Manufacturer:** METTLER TOLEDO **Model:** InLab Solids

**Serial No.:** 3065701 **ID.No.:** N/A

**Performance of Electrode system** (Three-Point Calibration at pH 4, 7 and 10)

Certified Value @25 °C (pH)	Average Indicator Reading		Relative Slope (%)	Uncertainty ( ± pH )	Coverage Factor ( k )
	pH	mV			
4.008	4.01	188	-	0.0071	2.00
7.001	7.00	13	98.9	0.0086	2.00
10.010	10.01	-160	97.2	0.0085	2.00
6.865	6.87	21	-	0.0074	2.00



## Calibration Report

**Certificate No.:** 2401718-001-01

**Equipment:** Digital Thermometer with RTD (pH Meter)

**Resolution:** 0.1 °C **Model:** SevenEasy pH  
**Serial No.:** 1231155210 **ID No.:** UAE.WAT.010/2553  
**Manufacturer:** METTLER TOLEDO

**Date of Calibration:** 11 March 2024

Page 4 of 5

**Location:** Chemical Calibration Laboratory, National Food Institute

**Environment Condition:**  
**Ambient Temperature** 23 °C ± 1 °C  
**Relative Humidity** 51 % ± 2 %

### Condition of this results of Calibration:

1. Calibration Method :
  - In house method: W-TE-025 by comparison with standard thermometer.
  - The Calibration is determined by comparing with a known temperature from a standard resistance thermometer.
  - The temperature scale in use at this laboratory is the International Temperature scale of 1990 ( ITS-90 ).

### 2. Reference Standard Instrument :

Instrument	Model	Serial No.	Certificate No.	Due Date	Through
HANDHELD THERMOMETER	1523	2118154	PSL-T 0877/66	06-Jun-24	TISTR
Platinum Resistance Thermometer (PRT)	5627A	877332			

Support Equipment : - Low Temperature Bath (ISOCAL-6), Model: Europa-6 Plus Basic, S/N: 341592/2

3. This certificate is traceable to International System of Units (SI Units).
4. This certificate was certified only for the instrument we calibrated.
5. This result of calibration was found accurate as shown on date and place of calibration only.

6. Condition of Calibrated Item : Good

7. Result of Calibration : ☒ Without adjustment ☐ After adjustment





## Calibration Report

**Certificate No.:** 2401718-001-01

**Equipment:** Digital Thermometer with RTD (pH Meter)

Resolution: 0.1 °C Model: SevenEasy pH

Serial No.: 1231155210 ID No.: UAE.WAT.010/2553

Manufacturer: METTLER TOLEDO

**Date of Calibration:** 11 March 2024

Page 5 of 5

**Calibration point:** 15.0, 25.0 and 35.0 °C

**Calibration result:**

- The probe was immersed in liquid bath or dry bath to a minimum depth of 100 mm.
- Description of probe, model : N/A S/N : N/A
- Dimension of probe : Diameter 4 mm., Length 120 mm.,
- Sheath material : Stainless Steel

UUC* Reading (°C)	Standard Temperature (°C)	Correction Value (°C)	Uncertainty ± (°C)
15.1	14.998	0.1	0.099
25.1	24.998	0.1	0.099
35.1	34.997	0.1	0.099

Note

- UUC\* : Unit Under Calibration

The report uncertainty of measurement was based on standard uncertainty multiplied by coverage factor k= 2, providing a level of confidence of approximately 95 %.

----- End -----



F-CS-012 Revision: 01 Date: 20-04-65





# Certificate of Calibration

**Equipment:** pH METER      Certificate No.: C07240167  
**Model:** SevenEasy      Issued Date: 9 April 2024  
**Serial No. (or ID.):** 1230525212 (UAE.WAS.003/2553)      Job No.: WO-00024208  
**Manufacturer:** METTLER TOLEDO      Page: 1 of 3  
**Electrode Serial No.:** 1156883      Model: InLab Solids      Brand: METTLER TOLEDO  
**Condition:** In Condition

**Customer:** United Analyst and Engineering Consultant Company Limited  
3 Soi Udomsuk 41 Sukhumvit Road,  
Bangkok, Prakanong, Bangkok 10260 Thailand

**Environment Condition:** Temperature 23 °C ± 2 °C  
Humidity 50 %RH ± 15 %RH

**Calibration Place:** Environment Laboratory, DKSH Technology Limited.  
2533 Sukhumvit Road, Bangchak,  
Phrakhanong, Bangkok 10260 Thailand


**Calibration By:** Miss.Orawan Khlaiphloi

**Calibration Date:** 9 April 2024

**The Method used:** In house method, CAL-WI-58, base on ASTM E 70-07

**Traceability:** This certificate is traceable to SI Units, Sample Test is assured through primary measurement method Harned cell, through CPAchem Ltd. (ISO/IEC 17034) Certificate No. 938377, 931985, 931984 And pH Scale traceable to the SI Units maintained by National Institute of Metrology (NIMT), Thailand through Industrial Foundation Electrical and Electronics Institute Certificate No. CA20230350EA

  
(Miss Orawan Khlaiphloi)  
Person in charge

  
(Mr. Nitinun Srihawan)  
Authorized signatory

This certificate is issued the units of measurement according to the International System of Units (SI). It provides traceability of measurement to international or national standard or other recognized national standard laboratories.

The measurement uncertainty stated is the expanded uncertainty which is obtained from the standard uncertainty multiplied by the coverage factor ( $k=2$ ) to provide a level of confidence of approximately 95%. It is determined in accordance with the Guide to Expression of Uncertainty in Measurement (GUM).

These results may be affected by deviations from specified conditions. The results relate only to the items tested, calibrated or sampled. The report shall not be reproduced except in full without approval of DKSH Technology Limited.

## Calibration Results:

### pH Scale

Input	pH Meter Reading			Uncertainty of Measurement (mV)	Coverage Factor (k)
	(mV)	Error (mV)	(pH)		
414.12	414	-0.12	0.00	0.58	2.00
354.96	355	0.04	1.00	0.58	2.00
295.8	296	0.20	2.00	0.58	2.00
236.64	237	0.36	3.00	0.58	2.00
177.48	178	0.52	4.00	0.58	2.00
118.32	118	-0.32	5.00	0.58	2.00
59.16	59	-0.16	6.00	0.58	2.00
0	0	0.00	7.00	0.58	2.00
-59.16	-59	0.16	8.00	0.58	2.00
-118.32	-118	0.32	9.00	0.58	2.00
-177.48	-177	0.48	10.00	0.58	2.00
-236.64	-236	0.64	11.00	0.58	2.00
-295.8	-296	-0.20	12.00	0.58	2.00
-354.96	-355	-0.04	13.00	0.58	2.00
-414.12	-414	0.12	14.00	0.58	2.00

**Practical slope and zero point\***

The three-point calibration using three standard buffer solutions; pH 4.008 , pH 6.985 and pH 9.997

-During calibration, display of pH meter reading; pH 4.00 , pH 7.00 and pH 10.01

The practical slope of the pH electrode; 57.01 (mV/pH), 96.37%

The zero point of the pH electrode; 6.88 (pH)

**Sample Test Results**

Standard Buffer Solution (pH)	Unit Under Calibration (pH)	Difference (pH)	Uncertainty of Measurement (pH)	Coverage Factor (k)
4.008	3.99	-0.018	0.0070	2.00
6.985	7.00	0.015	0.0091	2.00
9.997	10.02	0.023	0.0074	2.00

\* Calibration Marked " Not TISI Accredited " in this Certificate have been included for completeness.

**The End of Certificate**





## Certificate of Calibration

<b>Equipment:</b>	Digital Thermometer with Probe	<b>Certificate No.:</b>	C15240373
<b>Model:</b>	SevenEasy pH	<b>Issued Date:</b>	09 April 2024
<b>Serial No.:</b>	1230525212	<b>Job No.:</b>	WO-00024208
<b>Manufacturer:</b>	METTLER TOLEDO	<b>Page:</b>	1 of 2
<b>ID No.:</b>	UAE.WAS.003/2553	<b>Condition:</b>	In Condition

**Customer:** United Analyst and Engineering Consultant Company Limited  
3 Soi Udomsuk 41 Sukhumvit Road,  
Bangchak, Prakanong, Bangkok 10260 Thailand

**Environment Condition:** Temperature: 22 °C ± 3 °C  
Humidity: 50 %RH ± 20 %RH  
Voltage: 220 VAC ± 10 %

**Calibration Place:** Thermo-Hygro Laboratory, DKSH Technology Limited.  
2533 Sukhumvit Road, Bangchak,  
Phrakhanong, Bangkok 10260 Thailand

**Calibration By:** Mr. Nateekarn Mitjit

**Calibration Date:** 09 April 2024

**The Method used:** In house method, CAL-WI-19, by comparison with standard thermometer

**Traceability:** This certificate is traceable to the International System of Unit maintained by Quality Reborn Co.,Ltd. (QR) Certificate No. QR23-1073



(Mr. Nateekarn Mitjit)

Person in charge



(Mr. Pramote Ramrong)

Authorized signatory

This certificate is issued the units of measurement according to the International System of Units (SI). It provides traceability of measurement to international or national standard or other recognized national standard laboratories.

The measurement uncertainty stated is the expanded uncertainty which is obtained from the standard uncertainty multiplied by the coverage factor ( $k=2$ ) to provide a level of confidence of approximately 95%. It is determined in accordance with the Guide to Expression of Uncertainty in Measurement (GUM).

These results may be affected by deviations from specified conditions. The results relate only to the items tested, calibrated or sampled. The report shall not be reproduced except in full without approval of DKSH Technology Limited.

**Reference standard equipment:**

Equipment	Certificate no	Cal. date	Next Cal. date
Digital Thermometer with Probe	QR23-1073	2 May 23	2 May 24

**Calibration Results:****Without Adjustment**

Sensor Type: RTD

Channel: -


Diameter (mm) 4

Length (mm): 135

Immersion (mm): 110

Calibrate Point.(°C)	STD. Reading (°C)	UUC. Reading (°C)	Correction of UUC (°C)	Uncertainty (± °C)
15.0	15.010	15.1	-0.090	0.076
25.0	25.006	25.1	-0.094	0.076
35.0	35.004	35.0	0.004	0.076

**The End of Certificate**

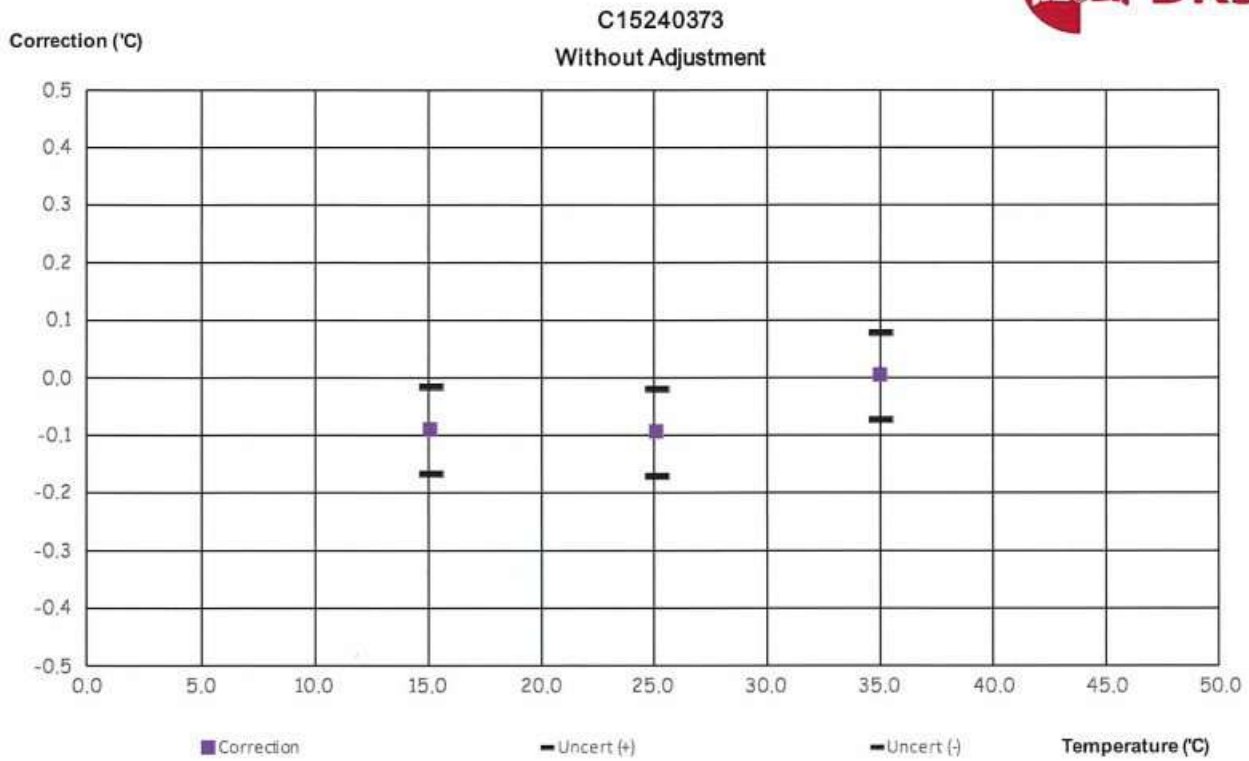



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)  
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES  
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250  
TEL. 0-2717-3000-29 FAX. 0-2719-9484



Cert. No.: 24TM303

Page : 1 of 3

## Certificate of Calibration

**Equipment :** BOD Incubator

**Manufacturer :** Arco

**Model :** UC4-1320

**Serial No. :** 13URC4S013201

**ID No. :** UAE.WAO.015/2561

**Submitted by :** United Analyst and Engineering Consultant Co.,Ltd.  
3 Soi Udomsuk 41, Sukhumvit Road,  
Bangchak, Phrakhanong,  
Bangkok 10260

**Location :** Lab Floor 2

**Received Order :** 10 February 2024

**Calibration Date :** 10 February 2024

**Ambient Temperature :** ( 26 ± 10 ) °C

**Relative Humidity :** ( 50 ± 30 ) %

**Calibrated by :** Tawatchai Pama

**Approved by :**

Approved Signatory

- ( ) Pornthippa Tameyakul  
( ☒ ) Unnopphol Harachai  
( ) Suwit Imjai

**Issue Date :**

19 February 2024

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written  
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

เอกสารไม่ควบคุม





Equipment : BOD Incubator  
Condition As-Received : Used Item  
Reference : 2402-0234OC-1  
**Result of Calibration :-** ( \* ) Without Adjustment  
Function of UUC\* : Temperature Source  
Fresh air setting : Not Available

Cert. No.: 24TM303

Page : 3 of 3

Calibration Point ( °C )	UUC* Setting ( °C )	UUC* Reading ( °C )	Temperature stability ( ± °C )	Temperature uniformity ( °C )	Overall Variation ( °C )	Coverage Factor <i>k</i>
20.0	20.1	19.9	0.37	0.72	1.4	2

Calibration Point ( °C )	Measured Temperature ( °C )									Uncertainty ( ± °C )
	Position									
	1	2	3	4	5	6	7	8	9 (ref.)	
20.0	19.873	19.803	20.322	19.690	19.615	19.585	19.612	19.558	19.645	0.58

**Average\*** : The average of 30 values in each position.

**Temperature stability** : One-half of the greatest maximum difference of measured temperature at any one sensor.

**Temperature uniformity** : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.

**Overall Variation** : The Difference of the maximum and minimum measured temperatures throughout observation.

**UUC\*** : Unit Under Calibration

Note : The reported uncertainty of measurement was included stability and excluded uniformity .

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

เอกสารไม่ควบคุม



**TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)**  
**CORPORATE SERVICES 3 : EQUIPMENT CALIBRATION AND TESTING SERVICES**


534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250

TEL. 0-2717-3000 FAX. 0-2719-9484

**Cert.No.:** 24TW39

**Page.:** 1 of 2

## Certificate of Testing

<b>Equipment :</b>	DO Meter
<b>Manufacturer :</b>	YSI
<b>Model :</b>	5100
<b>Serial No. :</b>	11B 101863
<b>ID No. :</b>	UAE.WAO.004/2554
<b>Received Date :</b>	20 February 2024
<b>Test Date :</b>	21 February 2024
<b>Reference :</b>	2402-0629DSC-1
<b>Submitted by :</b>	United Analyst and Engineering Consultant Co.,Ltd. 3 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
<b>Laboratory Condition :</b>	Temperature ( $25 \pm 5$ ) °C Humidity ( $50 \pm 20$ ) %
<b>Test Procedure :</b>	In - house method : CP-CH9 by Comparison Technique with Azide Modification Method
<b>Tested by :</b>	Walalak Sirithean
<b>Approved by :</b>	 Approved Signatory
( ) Pornthippa Tameyakul	
( ) Unnopphol Harachai	
(✓) Saithip Meangmai	
<b>Issue Date :</b>	22 February 2024

**เอกสารไม่ควบคุม**



Cert.No.: 24TW39

Page.: 2 of 2

**Condition of this result of calibration**

1. Reference Standard Instruments :

This certification is traceable to the International System of Unit through the reference standards laboratory of Industrial Calibration Center, Technology Promotion Association (Thailand-Japan).

<u>Instruments</u>	<u>Serial No.</u>	<u>ID No.</u>	<u>Certificate No.</u>	<u>Due Date</u>
1. Burette	-	130BU10	23CG1172	22 Mar 2025
2. Balance	14233821	110RC001	23MM405	16 July 2024

2. Standard Material :-

<u>Material</u>	<u>Manufacturer</u>	<u>Lot.No.</u>	<u>Assay</u>
Sodium Thiosulfate pentahydrate	Merck	AM1763316	100.2%

**Result :** Dissolved Oxygen Meter Adjustment With Air 100 %

Dissolved Oxygen Probe No.: 22B100125

<b>Titration Method (Azide Modification Method)</b> (mg/L)	<b>DO Meter Reading</b> (mg/L)	<b>Standard Deviation</b> (mg/L)
8.20	8.19	0.0055

This report was certified only for the instrument we tested. It is allowable to use for study  
Intend to use for advertising and referral purpose is prohibited. This report may not be reproduced  
other in full, without written approval of the laboratory

-o0o-

เอกสารไม่ควบคุม 





Equipment : BOD Incubator  
Condition As-Received : Used Item  
Reference : 2402-0234OC-1

Cert. No.: 24TM303

Page : 2 of 3

**Procedure Used :-**

Calibration were conducted using calibration procedure CP-OT02 based on TLAS G-20 according to direct measurement method with Data Acquisition which connected with Resistance Temperature Detector ( RTD ).

The temperature scale used was based on ITS-90.

**Condition of this result of calibration**

1. Reference standard instrument:-

<u>Instrument</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Traceable</u>	<u>Due Date</u>
1 ) Data Acquisition	MY59003411	23LM208	TPA	27 Dec 2024

2. This certificate is valid only to the item calibrated on date and place of calibration.


3. This certification is traceable to the International System of Unit.

**Remark :** TPA : Technology Promotion Association ( Thailand - Japan )

**Result of Calibration :-** ( \* ) Without Adjustment

**Function of UUC\* :** Temperature Source

**Fresh air setting :** Not Available

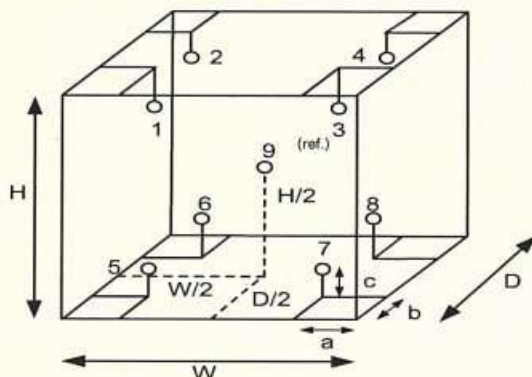

Environment during calibration		
	Beginning	Finished
Temp. ( °C )	28	31
REL.Humid. ( % )	70	65
AC Supply ( Volt )	233	234

Position :	Ref. Std. ID No.:
1	20RTD-2/1
2	20RTD-2/2
3	20RTD-2/3
4	20RTD-2/4
5	20RTD-2/5
6	20RTD-2/6
7	20RTD-2/7
8	20RTD-2/8
9 (ref.)	20RTD-2/9

**Probe Installation Details :**

a = 10 cm  
b = 10 cm  
c = 10 cm

**Dimension of Chamber :**

D = 0.62 m  
W = 1.2 m  
H = 1.2 m  
Capacity = 0.89 m<sup>3</sup>

เอกสารไม่ควบคุม



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)  
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES  
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250  
TEL.0-2717-3000-29 FAX.0-2719-9484



## Certificate of Calibration

Cert.No.: 24MM293

Page.: 1 of 3

**Equipment :** Electronic Balance

**Manufacturer :** Mettler Toledo

**Model :** XSR204

**Serial No. :** C117635043

**ID No. :** UAE.WAS.012/2564

**Submitted by :** United Analyst and Engineering Consultant Co.,Ltd.  
3 Soi Udomsuk 41, Sukhumvit Road,  
Bangchak, Phrakhanong,  
Bangkok 10260

**Location :** Balance Room (108)

**Received order :** 11 May 2024

**Calibration Date :** 11 May 2024

**Ambient Temperature :** 15 °C to 40 °C

**Relative Humidity :** 30 % to 90 %

**Calibrated by :** Khit Ruttanaprapachai

**Approved by :**   
Approved Signatory

( ) Ponpan Paipim  
( ) Suwit Imjai  
(✓) Kunchit Promprat

**Issue Date :** 15 May 2024

**The Uncertainties are for a confidence probability of approximately 95%**

This certificate may not be reproduced other than in full, except with the prior written  
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

เอกสารไม่ควบคุม



Equipment : Electronic Balance  
Condition As-Received : Used Item  
Reference : 2405-0166OC-2

Cert.No.: 24MM293

Page: 2 of 3

**Procedure used :-**

Calibration were conducted using in-house calibration procedure CP-OB01 based on UKAS LAB 14 according to direct measurement method against standard weight.

**Condition of this result of calibration**

1. Reference standard instruments:-

<u>Instruments</u>	<u>Model</u>	<u>Serial No.</u>	<u>ID No.</u>	<u>Test report No.</u>	<u>Due date</u>
1) Standard Weight Set (E2)	15884	24053	70RC007	MM-0013-24	25 Jan 2026

2. This certificate is valid only to the item calibrated on date and place of calibration.
3. This result of calibration was made on requested at the point specified by customer.
4. This certificate is not certified for any commercial transaction.
5. This certification is traceable to the International System of Unit.

**Result of calibration** ( ) Without Adjustment ( \* ) After Adjustment by Internal Calibration

**Range capacity :** 0 g to 220 g **Resolution** 0.0001 g

**Before Adjustment :**

<u>Applied Weight</u>	<u>Balance Reading</u>	<u>Correction</u>	<u>Measurement Uncertainty</u>	<u>Coverage Factor</u>
( g )	( g )	( g )	( ± mg )	( k )
100	100.0000	0.0000	0.27	2.03
200	200.0001	-0.0001	0.31	2

**After Adjustment :**

1. **Determination of the standard deviation of weighing machine** ( n = 10 )

<u>Applied Weight</u>	<u>Standard Deviation of Reading ( g )</u>
( g )	
100	0.00007
200	0.00007





Equipment : Electronic Balance  
Condition As-Received : Used Item  
Reference : 2405-0166OC-2


Cert.No.: 24MM293

Page: 3 of 3

### Result of calibration

#### 2. Effect of off center loading

A mass of 100 g was placed to various position on the pan.  
The weighing machine reading error obtained is given in the table

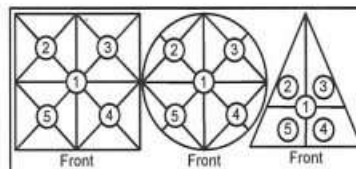

Maximum difference between  
off-center and central loading

Position 1 ( g )	Position 2 ( g )	Position 3 ( g )	Position 4 ( g )	Position 5 ( g )
+0.0002	-0.0001	0.0000	+0.0002	0.0000

( g )  
0.0003

#### 3. Departure from nominal value

Applied Weight ( g )	Balance Reading ( g )	Correction ( g )	Measurement Uncertainty ( ± mg )	Coverage Factor ( k )
Unload	0.0000	0.0000	0.15	2.13
1	1.0000	0.0000	0.15	2.13
5	5.0000	0.0000	0.15	2.13
10	10.0000	0.0000	0.15	2.11
20	20.0000	0.0000	0.19	2.03
50	50.0001	-0.0001	0.19	2.06
60	60.0001	-0.0001	0.19	2.04
80	80.0001	-0.0001	0.27	2
100	100.0002	-0.0002	0.27	2.03
120	120.0001	-0.0001	0.29	2
200	200.0001	-0.0001	0.31	2

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor  $k$ , providing a level of confidence of approximately 95 %.

-o0o-

## Calibration Certificate

**Certificate No.:** 2402283-002-01  
**Client name:** UNITED ANALYST AND ENGINEERING CONSULTANT CO., LTD.  
**Address:** 3 SOI UDOMSUK 41, SUKHUMVIT ROAD,  
Bangchack, Prakhonong, Bangkok 10260

Page 1 of 4

**Equipment:** Electronic Balance  
**Manufacturer:** METTLER TOLEDO  
**Model:** XSR205DU  
**Serial No.:** C210685394  
**ID No.:** UAE.WAO.010/2565  
**Order No.:** 2402283  
**Operation No.:** 2402283-002  
**Date of Receipt:** 2 April 2024  
**Date of Calibration:** 2 April 2024

**Calibrated by** Mr.Jerawut Prapawuttipong  
Scientist

**Approved by**



( Mr.Pheraphat Tuanjit )

Manager, Division of Calibration Laboratory

**Date of Issue:** 9 April 2024

Responsible for the Technical Management Team

**The uncertainties are for a confidence probability of approximately 95%**

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the National Food Institute.

F-CS-009 Revision: 01 Date: 20-04-65



## Calibration Report

**Certificate No.:** 2402283-002-01

**Equipment:**

Electronic Balance

**Manufacturer:** METTLER TOLEDO

**Model:** XSR205DU

**Resolution:** 0.00001 g / 0.0001 g

**Serial No.:** C210685394

**ID No.:** UAE.WAO.010/2565

**Capacity:** 220 g

**Date of Calibration:** 2 April 2024

Page 2 of 4

**Environment Condition:** Ambient Temperature: 24.5 ± 0.5 °C Relative Humidity: 47.5 ± 2.5 %

**Place of Calibration:** Laboratory, UNITED ANALYST AND ENGINEERING CONSULTANT CO., LTD.

**Condition of Equipment:** Good Condition

**Condition of This Results of Calibration:**

1. Calibration Method: NFI Method W-MA-001 In-House Method based on UKAS Lab 14 : 2019

2. Reference Standards:

Reference Standard	Model	Serial No.	Calibrated By	Certificate No.	Due Date
Standard Weight Class E2	1mg to 200g	B505567572	TCS	M2304053S	8 April 2024

Instrument	Model	Serial No.	Calibrated By	Certificate No.	Due Date
Thermo-Hygro Meter	608-H1	NFI.BTH 016/23	Quality Reborn	QR24-0343	9 February 2025

3. This certification is traceable to SI UNIT

4. This certificate was certified only for the instrument we calibrated.

5. This result of calibration was found accurate as shown on date and place of calibration only.

**Calibration Results:**




**1. Repeatability of Reading:**

Nominal Value ( g )	Standard Deviation of Reading ( g )
40	0.0000042
80	0.0000052
100	0.000048
200	0.000048

**2. Off-Center Error:**

A mass of 100 g was placed and moved to various position on pan.

The balance reading obtained is given in the table.



1	2	3	4	5	6	(Maximum Difference)
( g )	( g )	( g )	( g )	( g )	( g )	( g )
100.0000	100.0001	99.9999	99.9999	100.0001	100.0000	0.0001

*Handwritten signature*

F-CS-012 Revision: 01 Date: 20-04-65





## Calibration Report

**Certificate No.:** 2402283-002-01

**Equipment:**

Electronic Balance

**Manufacturer:** METTLER TOLEDO

**Model:** XSR205DU

**Resolution:** 0.00001 g / 0.0001 g

**Serial No.:** C210685394

**ID No.:** UAE.WAO.010/2565

**Capacity:** 220 g

**Date of Calibration:** 2 April 2024

Page 3 of 4

**Calibration Results:** (Continued)

**Calibration Range:** 0 - 80 g

**Calibration Adjustment:** Internal Calibration

**3. Departure from Nominal Value:** (Range: 0 - 80 g ; Resolution: 0.00001 g )

Nominal Value ( g )	Standard Value ( g )	Average Reading ( g )	Correction ( g )	Uncertainty ( ± g )	Coverage Factor k
Unload	0.000000	0.00000	0.00000	0.0000086	2.00
0.001	0.001003	0.00101	-0.00001	0.0000089	2.00
0.005	0.005003	0.00500	0.00000	0.0000092	2.00
0.01	0.010003	0.01000	0.00000	0.0000089	2.00
0.05	0.049996	0.05000	0.00000	0.0000096	2.00
0.1	0.100011	0.10000	0.00001	0.000011	2.00
0.5	0.500016	0.50001	0.00001	0.000014	2.00
1	1.000003	1.00002	-0.00002	0.000016	2.00
2	2.000023	2.00001	0.00001	0.000017	2.00
5	5.000017	5.00002	0.00000	0.000020	2.00
10	10.000009	10.00000	0.00001	0.000026	2.00
20	20.000031	20.00000	0.00003	0.000037	2.00
30	30.000040	30.00001	0.00003	0.000050	2.00
50	50.000028	50.00002	0.00001	0.000068	2.00
80	80.000068	80.00002	0.00005	0.00011	2.00



## Calibration Report

**Certificate No.:** 2402283-002-01

**Equipment:**

Electronic Balance

**Manufacturer:** METTLER TOLEDO

**Model:** XSR205DU

**Resolution:** 0.00001 g / 0.0001 g

**Serial No.:** C210685394

**ID No.:** UAE.WAO.010/2565

**Capacity:** 220 g

**Date of Calibration:** 2 April 2024

Page 4 of 4

**Calibration Results:** (Continued)

**Calibration Range:** 81 - 200 g

**Calibration Adjustment:** Internal Calibration

**3. Departure from Nominal Value:** (Range: 81 - 200 g ; Resolution: 0.0001 g )

Nominal Value ( g )	Standard Value ( g )	Average Reading ( g )	Correction ( g )	Uncertainty ( ± g )	Coverage Factor <i>k</i>
90	90.00010	90.0001	0.0000	0.00015	2.00
100	100.00006	100.0001	0.0000	0.00015	2.00
110	110.00007	110.0001	0.0000	0.00016	2.00
120	120.00009	120.0000	0.0001	0.00017	2.00
130	130.00010	130.0000	0.0001	0.00019	2.00
140	140.00014	140.0000	0.0001	0.00020	2.00
150	150.00009	150.0001	0.0000	0.00020	2.00
160	160.00010	160.0001	0.0000	0.00022	2.00
170	170.00012	170.0001	0.0000	0.00023	2.00
200	200.00016	200.0002	0.0000	0.00028	2.00

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k* , providing a level of confidence of approximately 95 %.

----- End -----



F-CS-012 Revision: 01 Date: 20-04-65



## Calibration Certificate

**Certificate No.:** 2500116-001-01  
**Client name:** UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.  
**Address:** 3 Soi Udomsuk 41, Sukhumvit Road,  
Bangchack, Prakhong, Bangkok 10260

Page 1 of 3

**Equipment:** CHAMBER (Hot Air Oven)

**Manufacturer:** MEMMERT

**Model:** UF55

**Serial No.:** B216.1666

**ID No.:** UAE.WAO.027/2559


**Order No.:** 2500116

**Operation No.:** 2500116-001

**Date of Receipt:** 8 October 2024

**Date of Calibration:** 8 October 2024

**Calibrated by** Mr.Yothin Charoensuk  
Scientist

**Approved by**   
( Mr.Pheraphat Tuanjit )

Manager, Division of Calibration Laboratory

**Date of Issue:** 15 October 2024

Responsible for the Technical Management Team

**The uncertainties are for a confidence probability of approximately 95 %.**

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the National Food Institute.

F-CS-009 Revision: 01 Date: 20-04-65



## Calibration Report

**Certificate No.:** 2500116-001-01

**Equipment:** CHAMBER (Hot Air Oven)

Model: UF55 Serial No.: B216.1666

Resolution: 0.1 °C ID No.: UAE.WAO.027/2559

Manufacturer: MEMMERT

**Date of Calibration:** 8 October 2024

Page 2 of 3

**Location:** Laboratory, UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.

**Environment Condition:**

Ambient Temperature ( 30.3 ± 1 ) °C

Relative Humidity ( 55 ± 1 ) %

Line Voltage ( 230 ± 3 ) Volt

### Condition of this results of Calibration:

- This instrument was calibrated by insert 9 standard thermometer into its chamber and calibration according to W-TE-014 Based on TLAS G-20-1/02-08 (E): Guidelines for Calibration and Checks of Temperature Controlled Enclosures.
  - The temperature scale used was based on ITS - 90.
  - All data show below were final values and the initial data may be obtained upon request.

### 2. Reference Standard Instrument :

Instrument	Model	Serial No./ID No.	Certificate No.	Due Date	Through
Digital Thermometer with sensor	34972A	MY57003188	TE 670486-01	8 June 2025	NATIONAL FOOD INSTITUTE
	RTD	CH#201-209/ RTD#201-209			

- This certificate is traceable to International System of Units (SI Units).
- This certificate was certified only for the instrument we calibrated.
- This result of calibration was found accurate as shown on date and place of calibration only.
- Condition of Calibrated item : Good

### UUC Description :

Time of Record 1 Hour 9 Minute At 104.0,140.0 and 180.0 °C

Fresh air Damper ☐ Open Position ☐

☒ Close Fan 40%

☐ Not Available

7. Result of Calibration : ☒ Without adjustment ☐ After adjustment






## Calibration Report

**Certificate No.:** 2500116-001-01

**Equipment:** CHAMBER (Hot Air Oven)

Model: UF55 Serial No.: B216.1666

Resolution: 0.1 °C ID No.: UAE.WAO.027/2559

Manufacturer: MEMMERT


**Date of Calibration:** 8 October 2024

Page 3 of 3

**Calibration point:** 104.0, 140.0 and 180.0 °C

**Calibration result:**

Calibration Condition	Temperature (°C)	Relative Humidity (%)	Line Voltage (Volt)
MIN	29.3	54	227.0
MAX	31.2	56	232.0

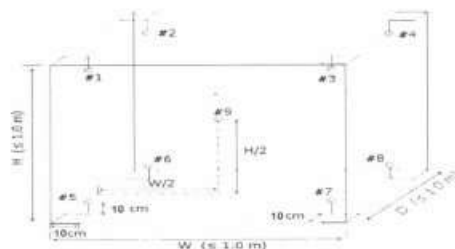

**Table 1 : Reporting of Temperature**

Calibration point (°C)	Measured Temperature (°C) @ Sensor No. (Sensor No.9 is REF)									Uncertainty ± (°C)
	# 1	# 2	# 3	# 4	# 5	# 6	# 7	# 8	# 9	
104.0	103.89	103.66	103.88	103.89	104.40	103.98	103.70	104.10	104.15	0.53
140.0	139.85	139.53	139.87	139.88	140.67	140.00	139.60	140.25	140.23	0.73
180.0	179.63	179.22	179.71	179.76	181.03	180.06	179.41	180.87	180.39	0.90

**Table 2 : Reporting of Characterization Result**

UUC* Setting (°C)	UUC* Reading (°C)			Stability ± (°C)	Uniformity (°C)	Overall Variation (°C)
	MIN	MAX	Average			
104.0	104.0	104.0	104.0	0.15	0.49	0.88
140.0	140.0	140.0	140.0	0.13	0.71	1.2
180.0	180.0	180.0	180.0	0.13	1.2	1.9

**Note** The quoted uncertainty include " Stability " and " Loading effect (20% of Temp Uniformity) "

UUC\* = Unit Under Calibration

Stability = One-half of the greatest maximum difference of measured temperatures at any one sensors, for at least half an hour after reaching steady state.

Uniformity = The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time.

Overall Variation = The difference of the maximum and minimum measured temperatures throughout observation time.

The report uncertainty of measurement was based on standard uncertainty multiplied by coverage factor  $k=2$ , providing a level of confidence of approximately 95 %.

----- End -----

*Handwritten signature*




Certificate No. : HIT-2417-0568

Page : 1 of 2

**CERTIFICATE OF CALIBRATION**

<b>Equipment :</b>	COD Test Tube Heater		
<b>Meter Model :</b>	HI839800-02	<b>Serial No. :</b>	1147807
<b>Tube Heater :</b>	25 Vial Capacity	<b>Resolution :</b>	0.1°C
<b>Temperature Range :</b>	(-10 to 160)°C	<b>Temperature of Reaction :</b>	150°C
<b>Manufacturer :</b>	Hanna Instruments	<b>Made in :</b>	Romania
<b>Condition As-Received :</b>	Used Product	<b>Reference :</b>	RE240681
<b>Ambient Temperature :</b>	(25 ± 2)°C	<b>Relative Humidity :</b>	(50 ± 15)%RH
<b>Customer name :</b>	United Analyst and Engineering Consultant Co., Ltd. 3 Soi Udomsuk 41, Sukhumvit Rd., Bangchak, Phrakhanong, Bangkok 10260		
<b>Received date :</b>	22 April 2024		
<b>Calibrate date :</b>	23 April 2024		
<b>Issue date :</b>	25 April 2024		
<b>Calibrated Location :</b>	Hanna Instruments (Thailand) Ltd.		
<b>Calibration Procedure :</b>	This calibrator was conducted by using in-house: calibration procedure CP-04 by using certified reference standard instruments.		

**Calibrated by :** ☒ Mr. Pichit Petthong  
☐ Mr. Channarong Soinak

**Approved by :**   
Mr. Anan Suwanchaisakul  
Authorized Signatory



This certificate was certified only for the instrument we calibrated.

This result of calibration was found accurate on date and place of calibration only.

\*\* This certificate may not be reproduced other than in full, except with the prior written \*\*  
approval of the head of Hanna Instrument (Thailand).

เอกสารไม่ควบคุม

### Condition of this calibration result:

Reference Standard Instruments : This certification is traceable to the international unit of unit maintained through:

Instruments	Model	Serial No.	Certificate No.	Traceable
Data Acquisition Switch Unit	34970A	MY44065265	WK2307-164-1	WK Electric Co., Ltd.
Digital Thermo-Hygrometer	HT-771SD	AI.07155	24H41	Technology Promotion Association (Thailand-Japan).

### Calibration Result:

Measurement Temperature Source Accuracy for COD Reactor.

Capacity (Vial)	Nominal Value (°C)	Average Value (°C)	Uncertainty of Measurement (±°C)
25 Vial	150.0	149.8	0.49

Unit : °C

(1A)	(2A)	(3A)	(4A)	(5A)
148.901	149.249	149.950	150.042	149.186
(1B)	(2B)	(3B)	(4B)	(5B)
149.724	149.578	149.852	150.100	150.117
(1C)	(2C)	(3C)	(4C)	(5C)
149.863	149.799	150.233	149.847	149.977
(1D)	(2D)	(3D)	(4D)	(5D)
149.550	149.666	149.958	149.744	149.819
(1E)	(2E)	(3E)	(4E)	(5E)
150.044	149.869	149.361	149.973	149.654

Figure: Shows the location of the temperature source.

The report uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor  $k = 2$ , providing a level of confidence of approximately 95%

**\*\* End of certificate \*\***



## Verification Certificate

**Substitute for Certificate No.:** 2402957-001-01  
**Certificate No.:** 2402957-001-02  
**Client name:** UNITED ANALYST AND ENGINEERING CONSULTANT CO., LTD.  
**Address:** 3 Soi Udomsuk 41, Sukhumvit Road,  
Bangchack, Prakhonong, Bangkok 10260

Page 1 of 4

**Equipment:** HEATING BLOCK DIGESTION  
**Manufacturer:** FOSS  
**Model:** 2520  
**Serial No.:** 91794469  
**ID No.:** UAE.WAS.011/2560  
**Order No.:** 2402957  
**Operation No.:** 2402957-001  
**Date of Receipt:** 23 May 2024  
**Date of Calibration:** 23-24 May 2024

**Calibrated by** Mr.Jerawut Prapawuttipong  
Scientist

**Approved by**

( Mr.Pheraphat Tuanjit )

Manager, Division of Calibration Laboratory

**Date of Issue:** 18 June 2024

Responsible for the Technical Management Team

**The uncertainties are for a confidence probability of approximately 95 %.**

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the National Food Institute.

F-CS-011 Revision: 01 Date: 20-04-65





## Verification Report

**Certificate No.:** 2402957-001-02  
**Equipment:** HEATING BLOCK DIGESTION  
Model: 2520 Serial No.: 91794469  
Resolution: 1 °C ID No.: UAE.WAS.011/2560  
Manufacturer: FOSS  
**Date of Calibration:** 23-24 May 2024

Page 2 of 4

**Location:** UNITED ANALYST AND ENGINEERING CONSULTANT CO., LTD.  
**Environment Condition:** Ambient Temperature ( 25 ± 3 ) °C  
Relative Humidity ( 55 ± 15 ) %  
Line Voltage ( 220 ± 10 ) Volt

### Condition of this results of Calibration:

- This instrument was calibrated by insert standard thermocouples type R into its heating block digestion and compared to temperature obtained from reference standards thermometer at calibrated point.
  - The temperature scale used was based on ITS - 90 .
  - All data show below were final values and the initial data may be obtained upon request.

### 2. Reference Standard Instrument :

Instrument	Model	Serial No.	Certificate No.	Due Date	Through
Digital Thermometer with Thermocouple	34970A	MY44045576/MY41194453	TC23/0048	2-Jun-2024	N.M. Technical Center Laboratory
	Type R	TC#101-103 / CH#101-103			

- This certificate is traceable to international system of units (SI Units).
- This certificate was certified only for the instrument we calibrated.
- This result of calibration was found accurate as shown on date and place of calibration only.
- Condition of Calibrated item : Good

UUC\* Description

Time of Record - Hour 30 Minute At 380 °C

7. Result of Calibration : ☒ Without adjustment ☐ After adjustment




## Verification Report

**Certificate No.:** 2402957-001-02  
**Equipment:** HEATING BLOCK DIGESTION  
Model: 2520 Serial No.: 91794469  
Resolution: 1 °C ID No.: UAE.WAS.011/2560  
Manufacturer: FOSS

**Date of Calibration:** 23-24 May 2024

Page 3 of 4

**Calibration point:** 380 °C

**Calibration result:**

### Reporting of Temperature

Block No.	UUC* Setting (°C)	UUC* Reading (°C)	Stability (±°C)	Standard Thermometer (°C)	Uncertainty (±°C)
1	380	380	0.96	378.86	2.1
2	380	380	0.40	378.41	2.1
3	380	380	1.18	378.94	2.1
4	380	380	0.44	377.64	1.6
5	380	380	0.11	377.75	1.6
6	380	380	0.14	378.35	1.6
7	380	380	1.17	377.09	2.1
8	380	380	0.33	377.08	2.1
9	380	380	0.14	376.61	2.1
10	380	380	0.96	377.74	2.1
11	380	380	0.40	377.17	2.1
12	380	380	1.18	377.71	2.1
13	380	380	0.44	379.07	1.6
14	380	380	0.11	379.19	1.6
15	380	380	0.14	379.78	1.6
16	380	380	1.17	378.74	2.1
17	380	380	0.33	378.74	2.1
18	380	380	0.14	378.27	2.1
19	380	380	0.96	379.53	2.1
20	380	380	0.40	378.96	2.1

### Note:

- UUC\* = Unit Under Calibration
- Immersion depth of standard thermometer in tube level high of sand is equal heater plate of UUC.
- Stability = One-half of the greatest maximum difference of measured temperatures at one sensors, for at least half an hour after reaching steady state.




## Verification Report

**Certificate No.:** 2402957-001-02

**Equipment:** HEATING BLOCK DIGESTION

Model: 2520      Serial No.: 91794469

Resolution: 1 °C      ID No.: UAE.WAS.011/2560

Manufacturer: FOSS


**Date of Calibration:** 23-24 May 2024

**Calibration point:** 380 °C

**Calibration result:** Continued

Page 4 of 4

Figure 1. Location of Reference Standard and Block Diagram of Digestion Unit

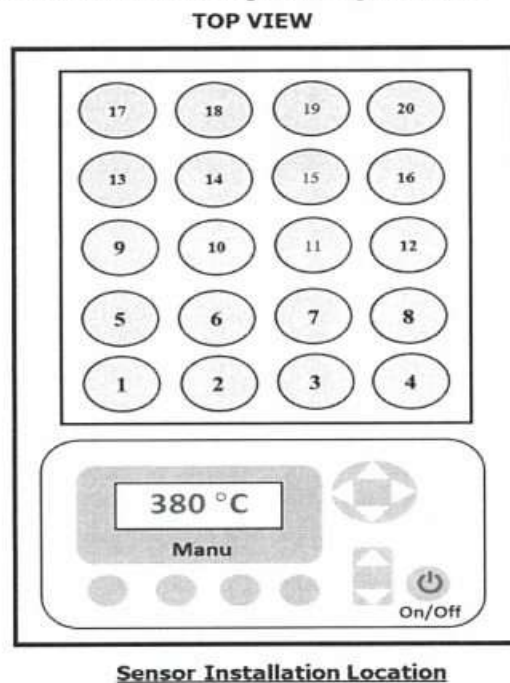

Remark: Edited Date of Calibration from 23-24 May 204 to 23-24 May 2024.

**Note:**

- UUC\* = Unit Under Calibration
- Immersion depth of standard thermometer in tube level high of sand is equal heater plate of UUC.
- Stability = One-half of the greatest maximum difference of measured temperatures at one sensors, for at least half an hour after reaching steady state.

The report uncertainty of measurement was based on standard uncertainty multiplied by coverage factor  $k=2$ , providing a level of confidence of approximately 95 %.

----- End -----

F-CS-012 Revision: 01 Date: 20-04-65



## เอกสารไม่ควบคุม

## เอกสารไม่ควบคุม



Request No. 25-67 / 0275

MTC. ACL.No. 358 / 67

## CALIBRATION CERTIFICATE

**NOMENCLATURE :** 1. Atomic Absorption Spectrophotometer "Agilent Technologies"

Model AA240FS, Serial No. MY13160001

2. Working standard solution "Inorganic Ventures"

Multi Analyte Custom Grade Solution, Lot No. S2-MEB675610

**SUBMITTED BY :** United Analyst and Engineering Consultant Co., Ltd.

3 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Prakanong, Bangkok 10260

**CALIBRATION PROCEDURE :** 1. Performance Verification of Atomic Absorption Spectrophotometer  
(WI-500-02-30)

2. Estimation Uncertainty of Measurement in Analytical Chemistry (QP-513)

**CALIBRATION RANGE:** 0.02, 0.10, 0.30, 0.50, 0.70 mg/l at 228.8 nm.Cd, 0.10, 0.20, 0.30, 0.50, 0.70 mg/l at 357.9 nm.Cr,  
0.05, 0.10, 0.30, 0.50, 0.70 mg/l at 324.7 nm.Cu, 0.10, 0.30, 0.50, 0.70, 1.00 mg/l at 248.3 nm.Fe,  
0.20, 0.50, 0.70, 1.00, 1.50 mg/l at 217.0 nm.Pb, 0.05, 0.10, 0.30, 0.50, 0.70 mg/l at 279.5 nm.Mn,  
0.10, 0.30, 0.50, 0.70, 1.00 mg/l at 232.0 nm.Ni, 0.05, 0.10, 0.30, 0.50, 0.70 mg/l at 213.9 nm.Zn

**CALIBRATION DATE :** 2 February 2024

**REFERENCE MATERIAL :** Traceable to NIST "Agilent Technologies", "CARLO ERBA"

Cadmium Lot No. 0006589926, Chromium Lot No. 0112384886, Copper Batch No. T117098A, Iron Batch No. T126087A,  
Lead Lot No. 1227873, Manganese Batch No. T109228A, Nickel Batch No. T270178A, Zinc Batch No. T820140A

**AMBIENT CONDITIONS :** Temperature  $25 \pm 5$  °C Relative humidity  $50 \pm 20$  %

The Atomic Absorption Spectrophotometer has been calibrated against Reference Material traceable to National Institute of Standards and Technology ( NIST ) by The Analytical Chemistry Laboratory. The results are attached herewith.

Calibrated by ..... Atipat .....

( Mr. Atipat Ratana )

Approved by ..... Sulda .....

(Miss Sutadde Deawtong)

Director of Analytical Chemistry Laboratory

Ref. 2015267020100454001

Issued Date : 11 March 2024

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.4

### Head Office

35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,  
Changwat Pathumthani 12120, Thailand  
Tel. (66) 0 2577 9000  
Fax. (66) 0 2577 9009  
E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

### Office/Laboratory

Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,  
Amphoe Muang, Changwat Samutprakan 10280, Thailand  
Tel. (66) 0 2323 1672-80 ext. 115, 116  
Fax. (66) 0 2323 9165  
E-mail : mtc@tistr.or.th

### Office

196 Phahonyothin Road, Chatuchak, Bangkok 10900,  
Thailand  
Tel. (66) 0 2579 8592  
Fax. (66) 0 2579 8592  
E-mail : sumalee@tistr.or.th

เอกสารไม่ควบคุม

# CALIBRATION DATA

## 1. Noise Level

Element	Cd	Cr	Cu	Fe	Pb	Mn	Ni	Zn
Absorbance	0.0006	0.0004	-0.0003	0.0001	-0.0011	-0.0005	0.0008	0.0004
	0.001	0.0017	-0.0009	0.0008	0.0001	0.0002	-0.0003	0.0007
	0.0006	0.0017	-0.0020	0.0005	0.0005	0.0004	0.0013	0.0014
	0.0001	0.0018	-0.0007	0.0005	0.0004	-0.0003	-0.0001	0.0010
	-0.0001	0.0019	-0.0014	0.0003	0.0010	0.0000	0.0002	-0.0001
	0.0011	0.0014	-0.0017	0.0009	-0.0008	0.0004	0.0006	0.0010
	-0.0002	0.0015	-0.0015	0.0003	0.0002	-0.0008	0.0009	0.0013
	0.0006	0.0012	-0.0001	0.0006	0.0008	0.0001	-0.0002	0.0013
	0.0008	0.0009	-0.0003	0.0003	0.0005	0.0002	0.0001	0.0007
	0.0012	0.0011	-0.0012	0.0008	0.0003	0.0004	0.0004	0.0013
	0.0003	0.0015	-0.0019	0.0001	-0.0002	0.0000	-0.0003	0.0003
	0.0005	0.0017	-0.0019	-0.0007	0.0000	-0.0007	0.0005	0.0005
	-0.0006	0.0016	0.0000	0.0006	-0.0001	0.0013	0.0006	0.0010
	0.0003	0.0011	-0.0002	0.0001	-0.0007	0.0009	0.0009	0.0002
	0.0003	0.0012	-0.0011	0.0007	-0.0003	-0.0003	0.0010	0.0009
	0.0004	0.0018	-0.0016	-0.0004	-0.0006	0.0008	0.0007	0.0007
	-0.0001	0.0018	-0.0018	0.0013	-0.0006	-0.0001	0.0014	0.0006
	0.0003	0.0017	-0.0001	0.0001	-0.0012	-0.0004	0.0001	0.0002
	0.0010	0.0018	-0.0007	0.0003	-0.0005	-0.0002	0.001	0.0003
	0.0004	0.0019	-0.0008	-0.0001	-0.0004	0.0003	0.0002	0.0008
Average Absorbance	0.000	0.001	-0.001	0.000	0.000	0.000	0.000	0.001

Continue 2 / 5

INDUSTRIAL METROLOGY AND TESTING SERVICE CENTRE

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.4

### Head Office

35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,  
Changwat Pathumthani 12120, Thailand  
Tel. (66) 0 2577 9000  
Fax. (66) 0 2577 9009  
E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

### Office/Laboratory

Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,  
Amphoe Muang, Changwat Samutprakan 10280, Thailand  
Tel. (66) 0 2323 1672-80 ext. 115, 116  
Fax. (66) 0 2323 9165  
E-mail : mtc@tistr.or.th

### Office

196 Phahonyothin Road, Chatuchak, Bangkok 10900,  
Thailand  
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217  
Fax. (66) 0 2519 8392  
E-mail : sumalee@tistr.or.th

เอกสารไม่ควบคุม




## 2. Precision

Element	Conc. (mg/l)	Absorbance										Ave. Abs.	SD	%RSD
Cd	0.02	0.0078	0.0076	0.0069	0.0075	0.0071	0.0070	0.0076	0.0074	0.0077	0.0067	0.007	0.0004	5.15
	0.30	0.1008	0.1007	0.0999	0.0997	0.1000	0.0996	0.1008	0.1002	0.1005	0.0999	0.100	0.0005	0.46
	0.70	0.2301	0.2306	0.2277	0.2305	0.2310	0.2295	0.2290	0.2293	0.2305	0.2296	0.230	0.0010	0.42
Cr	0.10	0.0094	0.0093	0.0093	0.0098	0.0094	0.0095	0.0090	0.0090	0.0094	0.0090	0.009	0.0003	2.75
	0.30	0.0241	0.0236	0.0221	0.0238	0.0231	0.0226	0.0231	0.0223	0.0230	0.0231	0.023	0.0006	2.75
	0.70	0.0500	0.0500	0.0500	0.0524	0.0499	0.0511	0.0509	0.0512	0.0515	0.0504	0.051	0.0008	1.63
Cu	0.05	0.0061	0.0062	0.0064	0.0061	0.0069	0.0069	0.0061	0.0062	0.0064	0.0061	0.006	0.0003	5.00
	0.30	0.0419	0.0411	0.0402	0.0407	0.0405	0.0404	0.0399	0.0400	0.0399	0.0400	0.040	0.0006	1.58
	0.70	0.0960	0.0960	0.0960	0.0959	0.0947	0.0955	0.0952	0.0952	0.0951	0.0955	0.096	0.0005	0.48
Fe	0.10	0.0096	0.0101	0.0103	0.0100	0.0099	0.0096	0.0106	0.0099	0.0105	0.0102	0.010	0.0003	3.38
	0.50	0.0424	0.0415	0.0428	0.0427	0.0421	0.0426	0.0413	0.0430	0.0421	0.0419	0.042	0.0006	1.33
	1.00	0.0830	0.0839	0.0847	0.0834	0.0832	0.0820	0.0839	0.0838	0.0837	0.0845	0.084	0.0008	0.92
Pb	0.20	0.0078	0.0074	0.0078	0.0078	0.0076	0.0078	0.0077	0.0078	0.0078	0.0077	0.008	0.0001	1.71
	0.70	0.0278	0.0273	0.0271	0.0267	0.0270	0.0264	0.0274	0.0273	0.0269	0.0269	0.027	0.0004	1.45
	1.50	0.0551	0.0548	0.0552	0.0555	0.0547	0.0546	0.0544	0.0544	0.0549	0.0547	0.055	0.0004	0.64
Mn	0.05	0.0116	0.0107	0.0110	0.0103	0.0108	0.0108	0.0112	0.0107	0.0109	0.0108	0.011	0.0003	3.15
	0.30	0.0650	0.0649	0.0649	0.0651	0.0646	0.0646	0.0649	0.0646	0.0640	0.0648	0.065	0.0003	0.48
	0.70	0.1463	0.1465	0.1459	0.1471	0.1475	0.1474	0.1487	0.1473	0.1462	0.1468	0.147	0.0008	0.56
Ni	0.10	0.0095	0.0100	0.0096	0.0103	0.0102	0.0096	0.0100	0.0095	0.0097	0.0096	0.010	0.0003	3.04
	0.50	0.0443	0.0433	0.0438	0.0444	0.0430	0.0437	0.0444	0.0437	0.0438	0.0434	0.044	0.0005	1.09
	1.00	0.0812	0.0820	0.0834	0.0829	0.0818	0.0829	0.0831	0.0835	0.0816	0.0819	0.082	0.0008	0.99
Zn	0.05	0.0374	0.0377	0.0373	0.0377	0.0374	0.0377	0.0373	0.0371	0.0371	0.0374	0.037	0.0002	0.61
	0.30	0.1985	0.1993	0.1975	0.1992	0.1979	0.1988	0.1995	0.1985	0.1974	0.2004	0.199	0.0009	0.47
	0.70	0.4027	0.4031	0.4019	0.4021	0.4023	0.3981	0.4042	0.4025	0.3993	0.3997	0.402	0.0019	0.48

Continue 3 / 5

INDUSTRIAL METROLOGY AND TESTING SERVICE CENTRE



The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.4

### Head Office

35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,  
Changwat Pathumthani 12120, Thailand  
Tel. (66) 0 2577 9000  
Fax. (66) 0 2577 9009  
E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

### Office/Laboratory

Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,  
Amphoe Muang, Changwat Samutprakan 10280, Thailand  
Tel. (66) 0 2323 1672-80 ext. 115, 116  
Fax. (66) 0 2323 9165  
E-mail : mtc@tistr.or.th

### Office

196 Phahonyothin Road, Chatuchak, Bangkok 10900,  
Thailand  
Tel. (66) 0 2579 5225, 5217  
Fax. (66) 0 2579 8592  
E-mail : sumalee@tistr.or.th

เอกสารไม่ควบคุม

Request No. 25-67 / 0275

3 / 5

MTC. ACL. No. 358 / 67

### 3. Trueness

#### 3.1 Reading on wavelength- Cadmium(Cd) at 228.8 nm.

Element	Standard Value of RM (mg/l)	Reading (mg/l)	Error of Measurement (mg/l)	Error of Measurement (%)	Uncertainty (mg/l)
Cd	0.020	0.020	0.000	1.10	± 0.005
	0.301	0.301	0.000	0.11	± 0.005
	0.707	0.693	-0.013	1.85	± 0.008

#### 3.2 Reading on wavelength- Chromium (Cr) at 357.9 nm.

Element	Standard Value of RM (mg/l)	Reading (mg/l)	Error of Measurement (mg/l)	Error of Measurement (%)	Uncertainty (mg/l)
Cr	0.1007	0.104	0.004	3.49	± 0.009
	0.3035	0.297	-0.006	2.11	± 0.012
	0.7071	0.685	-0.023	3.19	± 0.023

#### 3.3 Reading on wavelength- Copper (Cu) at 324.7 nm.

Element	Standard Value of RM (mg/l)	Reading (mg/l)	Error of Measurement (mg/l)	Error of Measurement (%)	Uncertainty (mg/l)
Cu	0.051	0.047	-0.004	7.58	± 0.003
	0.303	0.296	-0.007	2.19	± 0.009
	0.704	0.698	-0.005	0.74	± 0.020

*Sumalee*

Continue 4 / 5

INDUSTRIAL METROLOGY AND TESTING SERVICE CENTRE

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BLMTC.002 Rev.4

#### Head Office

35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,  
Changwat Pathumthani 12120, Thailand  
Tel. (66) 0 2577 9000  
Fax. (66) 0 2577 9009  
E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

#### Office/Laboratory

Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,  
Amphoe Muang, Changwat Samutprakan 10280, Thailand  
Tel. (66) 0 2323 1672-80 ext. 115, 116  
Fax. (66) 0 2323 9165  
E-mail : mtc@tistr.or.th

#### Office

196 Phahonyothin Road, Chatuchak, Bangkok 10900,  
Thailand  
Tel. (66) 0 2626 1378 ext. 5225, 5217  
Fax. (66) 0 2579 8592  
E-mail : sumalee@tistr.or.th

**เอกสารไม่ควบคุม**

Request No. 25-67 / 0275

4 / 5

MTC. ACL. No. 358 / 67

3.4 Reading on wavelength- Iron (Fe) at 248.3 nm.

Element	Standard Value of RM (mg/l)	Reading (mg/l)	Error of Measurement (mg/l)	Error of Measurement (%)	Uncertainty (mg/l)
Fe	0.100	0.104	0.005	4.60	± 0.014
	0.500	0.482	-0.018	3.55	± 0.016
	1.006	0.968	-0.038	3.75	± 0.029

3.5 Reading on wavelength- Lead (Pb) at 217.0 nm.

Element	Standard Value of RM (mg/l)	Reading (mg/l)	Error of Measurement (mg/l)	Error of Measurement (%)	Uncertainty (mg/l)
Pb	0.201	0.202	0.001	0.34	± 0.014
	0.706	0.719	0.012	1.73	± 0.030
	1.513	1.459	-0.054	3.57	± 0.061

3.6 Reading on wavelength- Manganese (Mn) at 279.5 nm.

Element	Standard Value of RM (mg/l)	Reading (mg/l)	Error of Measurement (mg/l)	Error of Measurement (%)	Uncertainty (mg/l)
Mn	0.0505	0.050	0.000	0.83	± 0.005
	0.3031	0.306	0.003	1.12	± 0.007
	0.7023	0.698	-0.004	0.62	± 0.014

*Sumalee*

Continue 5 / 5

INDUSTRIAL METROLOGY AND TESTING SERVICE CENTRE

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.4

Head Office

35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,  
Changwat Pathumthani 12120, Thailand  
Tel. (66) 0 2577 9000  
Fax. (66) 0 2577 9009  
E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

Office/Laboratory

Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,  
Amphoe Muang, Changwat Samutprakan 10280, Thailand  
Tel. (66) 0 2323 1672-80 ext. 115, 116  
Fax. (66) 0 2323 9165  
E-mail : mtc@tistr.or.th

Office

196 Phahonyothin Road, Chatuchak, Bangkok 10900,  
Thailand  
Tel. (66) 0 2579 8592  
Fax. (66) 0 2579 8592  
E-mail : sumalee@tistr.or.th

**เอกสารไม่ควบคุม**



Request No. 25-67 / 0275

5 / 5

MTC. ACL. No. 358 / 67

3.7 Reading on wavelength- Nickel (Ni) at 232.0 nm.

Element	Standard Value of RM (mg/l)	Reading (mg/l)	Error of Measurement (mg/l)	Error of Measurement (%)	Uncertainty (mg/l)
Ni	0.101	0.098	-0.003	2.90	± 0.013
	0.508	0.502	-0.006	1.16	± 0.018
	1.012	0.962	-0.051	5.02	± 0.032

3.8 Reading on wavelength- Zinc (Zn) at 213.9 nm.

Element	Standard Value of RM (mg/l)	Reading (mg/l)	Error of Measurement (mg/l)	Error of Measurement (%)	Uncertainty (mg/l)
Zn	0.050	0.045	-0.005	9.39	± 0.013
	0.303	0.324	0.021	7.04	± 0.013
	0.707	0.675	-0.032	4.52	± 0.019

Remark : The reported uncertainty is an expanded uncertainty calculated using a coverage factor of 2 ( $k = 2$ ) which gives a level of confidence of approximately 95%

Calibrated by ..... Atipat .....

(Mr. Atipat Ratana)

Approved by ..... Sul Da .....

(Miss Suladda Deawtong)

Director of Analytical Chemistry Laboratory

Issued Date : 11 March 2024

INDUSTRIAL METROLOGY AND TESTING SERVICE CENTRE

End of Certificate

The results relate only to the items tested/calibrated or value assigned.  
Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.4

Head Office

35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,  
Changwat Pathumthani 12120, Thailand

Tel. (66) 0 2577 9000

Fax. (66) 0 2577 9009

E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

Office/Laboratory

Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,  
Amphoe Muang, Changwat Samutprakan 10280, Thailand

Tel. (66) 0 2323 1672-80 ext. 115, 116

Fax. (66) 0 2323 9165

E-mail : mtc@tistr.or.th

Office

196 Phahonyothin Road, Chatuchak, Bangkok 10900,  
Thailand

Tel. (66) 0 2579 8592

Fax. (66) 0 2579 8592

E-mail : sumalee@tistr.or.th

เอกสารไม่ควบคุม

## Agilent CrossLab Start Up Services

### Agilent 5100 5110 ICP-OES Preventive Maintenance



Agilent Preventive Maintenance provides factory recommended service for your analytical instruments to assure reliable operation and the accuracy of your results

Delivered by highly trained and certified service engineers using genuine Agilent parts and supplies, Agilent Preventive Maintenance provides what you need to reduce unplanned downtime and keep your systems operating at their peak performance.

This checklist is used as a guide for completing the preventive maintenance tasks. A signed copy of this checklist is provided for your records.

## Introduction

### Customer Information

- Customers should provide all necessary operating supplies upon request of the engineer.
- A customer representative should be available to the engineer while performing the preventive maintenance procedures. Customers are responsible for regular maintenance and are encouraged to observe the service representative.
- Any parts not included in the Parts Lists section of this document are not part of the recommended Preventive Maintenance service nor are they included in the price of this service.
- If a system requires the use of extra or special procedures and/or parts for the maintenance service, then these must be ordered separately and charged as a repair, which may incur additional costs.
- For customers using HF applications, the instrument should be returned to its standard sample introduction system.

## Important Customer Web Links

- To access **Agilent University**, visit <http://www.agilent.com/crosslab/university/> to learn about training options, which include online, classroom and onsite delivery. A training specialist can work directly with you to help determine your best options.
- To access the **Agilent Resource Center** web page, visit <https://www.agilent.com/en-us/agilentresources>. The following information topics are available:
  - Sample Prep and Containment
  - Chemical Standards
  - Analysis
  - Service and Support
  - Application Workflows
- The **Agilent Community** is an excellent place to get answers, collaborate with others about applications and Agilent products, and find in-depth documents and videos relevant to Agilent technologies. Visit <https://community.agilent.com/welcome>
- Videos about specific preparation requirements for your instrument can be found by searching the **Agilent YouTube** channel at <https://www.youtube.com/user/agilent>
- **Need to place a service call?** [Flexible Repair Options | Agilent](#)



## Service Engineer's Responsibilities

- Contact the customer and ensure that all necessary supplies are available before the preventive maintenance visit.
- Only select those pages that relate to the system or module being serviced.
- Complete empty fields with the relevant information.
- Complete the relevant checkboxes in the checklist using either a "X" or tick mark "✓".
- Check **"Service not applicable"** check boxes to indicate services/tasks not delivered, as appropriate.
- Complete the Preventive Maintenance services in the most logical order relevant to the individual system service in the order of the tasks listed.
- Complete the **Service Review** section together with the customer.
- Complete the fields for page numbers at the foot of each selected page
- Add relevant page numbers to selected pages and complete the total number of pages field in the Service Completion section
- **Ask the customer to sign the Service Verification section including the customer's and your signature.**



## Instrument Maintenance

### System Information

- ☐ Check this box if an instrument configuration report is attached instead of completing the table.

Instrument System Name and ID	5110 VDV ICP-OES
Instrument System Site and Location	United Analyst and Engineering Consultant

List System Component Product Numbers	List the Serial Numbers of each Component
1. G 8015A	MY 18030001
2.	
3.	
4.	
5.	
6.	
7.	
8.	
9.	

ICP-OES Configuration Table	Circle the type or write in the type if other
Nebulizer Type	SeaSpray (OneNeb) Conikal   Other
Spray Chamber	Cyclonic Single Pass (Cyclonic Double Pass) Other
Torch	Radial (Dual View) Other
Torch Type	One Piece (Semi Demountable) Fully Demountable   Other
Injector Diameter	2.4mm (1.8mm) 1.4mm   0.8mm   Other
Injector Material	(Quartz) Ceramic   Other

## Preparation

- ☒ Discuss any specific issues with the customer before starting.
- ☒ Review the instrument logbook for recorded problems and comments.
- ☒ Save instrument control settings before starting the procedure.
- ☒ Perform a general inspection of the system for cleanliness.
- ☒ Check for proper installation of parts, assemblies, sensors etc.
- ☒ Check system for required installation of components and implementation of Service Notes
- ☒ Check for required firmware/software updates and verify with customers if they would like them installed.
- ☐ For HF application systems, if standard sample introduction system was not installed, ask the customer to install it. ๙๑๖
- ☒ Ask the customer to remove any samples from the ICP-OES sample introduction area, auto sampler or around the ICP-OES.

## Preventive Maintenance Procedures

### Record Pre-PM instrument performance

- ☒ Run Instrument Performance test.
- ☒ Record results in Instrument Performance Test Results Table – Pre-PM.

### Clean and inspect ICP-OES system

- ☒ Look for any obvious external damage or problems.
- ☒ Inspect water cooling hoses, gas lines and power cord for excessive wear or damage.
- ☒ Perform a general internal inspection of the system for excessive dust accumulation, clean if necessary.
- ☒ Inspect sample introduction components and record any required maintenance in the Service Engineer Comments and notify the customer as the required actions required.
- ☒ Record the instrument operating conditions in the ICP-OES Status Results Table.
- ☒ Replace the polychromator purge filter.
- ☒ Replace the radial pre-optics window
- ☒ Replace the axial pre-optics window for SVDV and VDV instruments.
- ☒ Check exhaust flow for the correct positive extraction at the exhaust duct to insure they meet minimum specifications.
- ☒ Replace air inlet dust filter.
- ☐ Replace high capacity air inlet dust filter element if installed. N/A
- ☒ Remove and clean instrument water inlet filter.

### Agilent Water Recirculator

- ☐ **Service not applicable**
- ☒ Drain cooling fluid and remove any particles from the chiller reservoir
- ☒ Remove, clean and reinstall water inlet metal mesh filter if present.
- ☒ Re fill with Agilent Cool Clear cooling fluid.
- ☒ Clean the cooling system Air filter and the condenser.

### SPS 3 Auto Sampler

- ☒ **Service not applicable**
- ☐ Power cycle the autosampler and verify successful initialization.
- ☐ Inspect X and Z axis belts for wear. Replace is necessary.
- ☐ Clean X and Z axis slide shafts.
- ☐ Using customer's racks and the Agilent software move the sample probe to the 4 outermost corners and rinse port, ensure that the probe is approximately centered in the vial.

### SPS 4 Auto sampler

- ☒ **Service not applicable**
- ☐ Clean the spill tray, rack location mat, end frames and chassis with a damp soft cloth and diluted mild detergent.
- ☐ Clean the auto sampler cover panels, if cover kit is installed, with domestic window cleaner.
- ☐ Check the X-axis and Z-axis drive belts for cracks, splits, damaged teeth, excessive fraying, color changes or degradation from fumes.
- ☐ Check the X-axis, Theta-axis and Z-axis FFC cables for cracks, incorrect positioning, damaged edges or damaged connectors.
- ☐ Pump Tubing Replacement. Replace peristaltic pump tubing. Replace all tubing that goes from the rinse station to the pump and from the pump to the waste/rinse bottles
- ☐ Test using customer's tray and move the sample probe to the sample vial 1, wash vial and rinse port and ensure that the probe is centered in the vial. If not use calibration wizard and calibrate the position.

### AVS 4, 6, 7 Advanced Valve System

- ☒ **Service not applicable**
- ☐ Replace valve rotor seal
- ☐ Check fittings for signs of leaks
- ☐ Check tubing including autosampler tubing for kinks or excessive wear
- ☐ Check high flow pump for signs of leaks



## ICP-OES adjustment

- ☒ Check position of Zn peak, adjust if required.
- ☒ Check Argon Ratio, adjust to specified value if required.
- ☒ Perform Detector Calibration.
- ☒ Perform Instrument Calibration.

## Record Post-PM instrument performance

- ☒ Run Instrument Performance test.
- ☒ Record results in Instrument Performance Test Results Table - Post PM.
- ☒ For systems using ICP Expert version 7.3 and above, run the following Instrument tests
  - ☒ Subsystem Communications Test
  - ☒ Air Flow
  - ☒ Water Flow
  - ☒ Gas Flows
  - ☒ RF Generator
  - ☒ Camera Test
  - ☒ Optics Test
  - ☒ Nebulizer Test
- ☒ Record the result in the Instrument Test Results Table



## Restore Instrument

- ☐ For HF applications, ask the customer to reinstall their sample introduction system. N/A
- ☒ Leave system in an idle state: on and purging.
- ☒ Guidance: If the PM service is performed prior to a qualification service, then use the qualification procedure as a guide for final instrument set up and checkout.

## Service Review

- ☒ Attach available reports/printouts of all tests to this documentation.
- ☒ Record the Preventive Maintenance service activity in the customer's records/logbook.
- ☒ Record the PM event in the Smart Alerts logbook, if applicable.
- ☒ Update/reset instrument maintenance counters as appropriate.
- ☒ Affix the PM sticker to the system or instrument logbook based on the customer's request.
- ☒ Complete the Service Engineer Comments section if there are additional comments.
- ☒ Review this service, parts replaced, and test results obtained with the customer.
- ☒ If the instrument firmware was updated, record the details of the change in the Service Engineer's Comments box. Systems in a compliant environment may need additional documentation.
- ☒ **Complete the Signature Page with both Service Engineer and Customer signatures.**

## Test Results

### Instrument Performance Test Results Table

Note: These measurements do not form part of any specification and are for reference only.

	Pre PM Sensitivity Check		Post PM Sensitivity Check	
	Radial	Axial *	Radial	Axial*
Zn 213.857 nm SRBR	1500.8	2217.4	4124.8	6965.9
Mn 257.610 nm SRBR	3915.0	7492.2	13017.8	31121.6
Al 396.152 nm SBR	7.7	10.7	9.7	21.1
K 766.491 nm SBR	5.7	28.1	4.8	45.3

\* Axial result is not applicable for G8016AA, G8012AA Radial View instruments.

### Instrument Test Results Table

Note: The Instrument Test results are for systems using ICP Expert version 7.3 and above only.

Instrument Test	Result
Subsystem Communications Test	Pass
Air Flow	Pass
Water Flow	Pass
Gas Flows	Pass
RF Generator	Pass
Camera Test	Pass
Optics Test	Pass
Nebulizer test	Pass

## ICP-OES Status Results Table

Note: These measurements do not form part of any specification and are for reference only.

Measurement	Standby Mode		Plasma On	
Mains Voltage	231.411	VAC	226.871	VAC
Mains Current	0.081	A	0.105	A
Instrument Temperature	22.1	°C	23.5	°C
RF Air Flow (sensor speed)	14.0	Hz	19.0	Hz
Plasma Exhaust Temperature	No measurement		63.8	°C
Water Flow Oscillator	No measurement		1.34	L/min
Water Flow Detector	0.86	L/min	0.81	L/min
Water Inlet Temperature	19.7	°C	19.7	°C
Polychromator Temperature	35.0	°C	35.0	°C
CCD Temperature	-40.1	°C	-39.8	°C
Thermal Stabilizer	35.0	°C	35.0	°C
Argon Supply Pressure	648.92	kPa	591.55	kPa
Purge Gas Supply Pressure*1	646.66	kPa	612.41	kPa
Option Gas Supply Pressure*1	-	kPa	-	kPa
Nebulizer Flow	No measurement		0.70	L/min
Nebulizer Back Pressure	No measurement		158.43	kPa
Plasma Gas Flow	No measurement		11.91	L/min
Auxiliary Gas Flow	No measurement		1.00	L/min
RF Power	No measurement		1204.7	W
RF Supply Current	No measurement		7.858	A
RF Supply Voltage	No measurement		204.417	V

\*1 If option installed

## Consumed PM Parts

Part Description	Part Number	Product or Model# where used	Quantity consumed
Axial Pre-Optic Window	G8010-68014	G8010A, G8011A, G8014A/G8015A	1
Radial Pre-Optic Window	G8010-68015	All	1
Agilent Cool Clear Coolant Fluid	5799-0037	Agilent Water Recirculator	-
Purge Gas Filter	G8010-60136	All	1
Air inlet filter	G8000-68002	All	1
High Capacity Air Filter	G8010-60189	Optional	-
Rotor seal for 6-7 port valve for AVS6/7	G8494-60002	G8494A/G8495	-
Rotor seal for 4 port valve for AVS4	G8493-60002	G8493A	-
Rinse solution to rinse station 2.5mm id x 1m	G8410-80123	SPS 4	-
Barb connector 2.5mm-1.5mm ID	G8410-80124	SPS 4	-
PVC waste tubing, 8mm od x 5mm id, 2m	G8410-80122	SPS 4	-
<b>Additional Parts may be required from engineer's stock:</b>			
X axis drive belt	5410047500	SPS 3	-
Z axis drive belt	5410047400	SPS 3	-
Peristaltic pump tubing, PVC SolvaFlex, 3 bridged,	3710049000	SPS 4	-

## Consumed Parts Reference (Purchased by customer, not included as part of PM)

☒ Section Not Applicable.

Part Description	Part Number	Product or Model# where used	Quantity consumed



## Signature Page

### Service Engineer Comments (optional)

If there are any specific points you wish to note as part of performing the installation or other items of interest for the customer, please write in this box.

## Service Verification

Service Request Number:

6007197100

Service Engineer Name:

Kanyakorn S.

Service Engineer Signature:

Kanyakorn S.

Total number of pages in this document:

14

Date Service Completed:

04 Nov 2024

Customer Name:

Aphorn Onkong

Customer Signature:

Aphorn Onkong



**Report Summary**

Instrument Model	Agilent 5100/5110 VDV ICP-OES
Instrument ID	G8011A/G8015A
Instrument Serial Number	MY18030001
Software Version	7.3.1.9507
Firmware Version	3442
Tested By	Pre Test_PM_Kanyakorn S.
Test Completed On	11/4/2024 9:19:10 AM

**Result Summary**

Subsystem Communications Test	Skipped
Air Flow Test	Skipped
Water Flow Test	Skipped
Gas Flows Test	Skipped
RF Generator Test	Skipped
Camera Test	Skipped
Optics Test	Skipped
Advanced Valve System Test	Skipped
Resolution Test	Pass
Sensitivity Test	Fail
Precision Test	Pass

**Resolution Test****Pass**

Element Wavelength	Specification	Width
N (174.213 nm)	≤ 9.40	6.98
As (188.980 nm)	≤ 8.20	6.17
C (193.027 nm)	≤ 11.50	8.30
Mo (202.032 nm)	≤ 8.20	6.38
Cr (206.158 nm)	≤ 13.40	8.98
Zn (213.857 nm)	≤ 8.70	6.60
Pb (220.353 nm)	≤ 9.50	7.09
Co (228.615 nm)	≤ 17.20	11.67
Ba (230.424 nm)	≤ 9.40	7.20
Mn (257.610 nm)	≤ 13.30	9.43
Mn (260.568 nm)	≤ 20.30	14.11
Cr (267.716 nm)	≤ 11.00	8.04
Cu (324.754 nm)	≤ 25.00	18.97
Cu (327.395 nm)	≤ 14.20	11.23
Sr (338.071 nm)	≤ 33.50	24.30
Ba (455.403 nm)	≤ 44.00	33.47
Sr (460.733 nm)	≤ 36.00	17.23
Ba (493.408 nm)	≤ 36.00	25.37
Ba (614.171 nm)	≤ 42.00	25.54
Ar (675.283 nm)	≤ 74.00	56.51
K (766.491 nm)	≤ 80.00	65.86

**Sensitivity Test****Fail****Radial**

Element Wavelength	Specification	Method	Ratio	Standard	Blank
As (188.980 nm)	≥ 46.0	SRBR	104.1	793.0	50.8
Se (196.026 nm)	≥ 41.0	SRBR	87.6	862.0	79.7
Zn (213.857 nm)	≥ 1421.0	SRBR	1500.8	41823.3	749.0
Pb (220.353 nm)	≥ 46.0	SRBR	170.7	2432.0	174.9
Mn (257.610 nm)	≥ 3518.0	SRBR	3915.0	264700.2	4420.0
Al (396.152 nm)	≥ 3.4	SBR	7.7	48454.6	5563.2
Ba (493.408 nm)	≥ 34.0	SBR	45.9	1966719.7	41903.8
K (766.491 nm)	≥ 1.8	SBR	5.7	99036.2	14687.7

**Axial**

Element Wavelength	Specification	Method	Ratio	Standard	Blank
As (188.980 nm)	≥ 208.0	SRBR	126.5	1498.8	119.0
Se (196.026 nm)	≥ 159.0	SRBR	112.0	1773.6	197.8
Zn (206.200 nm)	≥ 234.0	SRBR	466.0	6784.2	199.7
Zn (213.857 nm)	≥ 1743.0	SRBR	2217.4	95597.6	1789.7
Cd (214.439 nm)	≥ 4227.0	SRBR	1919.3	68724.6	1236.4
Pb (220.353 nm)	≥ 320.0	SRBR	332.6	7929.5	499.0
Mn (257.610 nm)	≥ 10625.0	SRBR	7492.2	991238.3	16911.7
Cr (267.716 nm)	≥ 1048.0	SRBR	2254.6	129706.6	3150.9
Cu (324.754 nm)	≥ 19.0	SBR	26.9	290746.3	10407.5
Al (396.152 nm)	≥ 6.0	SBR	10.7	211329.2	18005.0
Ba (493.408 nm)	≥ 60.0	SBR	49.3	6956460.4	138336.9
K (766.491 nm)	≥ 24.0	SBR	28.1	1395190.2	47996.2

**Precision Test****Pass****Radial**

Element Wavelength	Specification	Measured Value % RSD
As (188.980 nm)	$\leq 2.60$	0.73
Se (196.026 nm)	$\leq 2.60$	0.95
Zn (213.857 nm)	$\leq 1.50$	0.31
Pb (220.353 nm)	$\leq 2.60$	0.73
Mn (257.610 nm)	$\leq 1.50$	0.39
Al (396.152 nm)	$\leq 1.50$	0.39
Ba (493.408 nm)	$\leq 1.50$	0.87
K (766.491 nm)	$\leq 1.50$	0.32

**Axial**

Element Wavelength	Specification	Measured Value % RSD
As (188.980 nm)	$\leq 1.50$	1.21
Se (196.026 nm)	$\leq 1.50$	0.84
Zn (206.200 nm)	$\leq 1.50$	0.56
Zn (213.857 nm)	$\leq 1.50$	0.96
Cd (214.439 nm)	$\leq 1.50$	0.26
Pb (220.353 nm)	$\leq 1.50$	0.51
Mn (257.610 nm)	$\leq 1.50$	0.97
Cr (267.716 nm)	$\leq 1.50$	0.22
Cu (324.754 nm)	$\leq 1.50$	0.24
Al (396.152 nm)	$\leq 1.50$	0.33
Ba (493.408 nm)	$\leq 1.50$	0.40
K (766.491 nm)	$\leq 1.50$	0.65

### Report Summary

Instrument Model	Agilent 5100/5110 VDV ICP-OES
Instrument ID	G8011A/G8015A
Instrument Serial Number	MY18030001
Software Version	7.3.1.9507
Platform	3442
Tested By	Post Test_PM_Kanyakorn S.
Test Completed On	11/4/2024 11:07:24 AM

### Result Summary

Subsystem Communications Test	Pass
Air Flow Test	Skipped
Water Flow Test	Skipped
Gas Flows Test	Skipped
RF Generator Test	Skipped
Camera Test	Skipped
Optics Test	Pass
Advanced Valve System Test	Skipped
Resolution Test	Pass
Sensitivity Test	Fail
Precision Test	Pass
Subsystem Communications Test	Pass

### Optics Test

	Radial	Axial
Intensity	3184054	3177175
Wavelength	737.212	737.212



Resolution Test		Pass
Element Wavelength	Specification	Width
N (174.213 nm)	≤ 9.40	6.97
As (188.980 nm)	≤ 8.20	6.14
C (193.027 nm)	≤ 11.50	8.33
Mo (202.032 nm)	≤ 8.20	6.33
Cr (206.133 nm)	≤ 13.40	9.06
Zn (213.637 nm)	≤ 8.70	6.70
Pb (220.353 nm)	≤ 9.50	7.03
Co (228.615 nm)	≤ 17.20	11.72
Ba (230.424 nm)	≤ 9.40	7.32
Mn (257.610 nm)	≤ 13.30	9.44
Mn (260.568 nm)	≤ 20.30	14.21
Cr (267.716 nm)	≤ 11.00	7.94
Cu (324.754 nm)	≤ 25.00	18.99
Cu (327.395 nm)	≤ 14.20	11.27
Sr (338.071 nm)	≤ 33.50	24.40
Ba (455.403 nm)	≤ 44.00	33.50
Sr (460.733 nm)	≤ 36.00	17.31
Ba (493.408 nm)	≤ 36.00	25.44
Ba (614.171 nm)	≤ 42.00	25.16
Ar (675.283 nm)	≤ 74.00	56.15
K (766.491 nm)	≤ 80.00	65.56

## Sensitivity Test

Fail

## Radial

Element Wavelength	Specification	Method	Ratio	Standard	Blank
As (188.980 nm)	≥ 46.0	SRBR	130.6	977.1	50.4
Se (196.026 nm)	≥ 41.0	SRBR	106.0	958.7	70.2
Zn (213.857 nm)	≥ 1421.0	SRBR	4124.8	44037.7	113.4
Pb (220.353 nm)	≥ 46.0	SRBR	207.2	2554.7	136.2
Mn (257.610 nm)	≥ 3518.0	SRBR	13017.8	271846.6	434.7
Al (396.152 nm)	≥ 3.4	SBR	9.7	50615.5	4717.0
Ba (493.408 nm)	≥ 34.0	SBR	133.7	2069203.0	15359.3
K (766.491 nm)	≥ 1.8	SBR	4.8	100199.5	17235.5

## Axial

Element Wavelength	Specification	Method	Ratio	Standard	Blank
As (188.980 nm)	≥ 208.0	SRBR	174.9	1566.7	73.0
Se (196.026 nm)	≥ 159.0	SRBR	167.0	1863.4	110.2
Zn (206.200 nm)	≥ 234.0	SRBR	740.9	6836.0	83.1
Zn (213.857 nm)	≥ 1743.0	SRBR	6965.9	101568.1	211.7
Cd (214.439 nm)	≥ 4227.0	SRBR	5781.0	72852.9	158.1
Pb (220.353 nm)	≥ 320.0	SRBR	501.0	8464.3	267.7
Mn (257.610 nm)	≥ 10625.0	SRBR	31121.6	1006637.8	1044.0
Cr (267.716 nm)	≥ 1048.0	SRBR	4424.8	132202.9	880.8
Cu (324.754 nm)	≥ 19.0	SBR	68.7	302907.8	4345.6
Al (396.152 nm)	≥ 6.0	SBR	21.1	218771.0	9892.3
Ba (493.408 nm)	≥ 60.0	SBR	250.6	7137380.9	28367.3
K (766.491 nm)	≥ 24.0	SBR	45.3	1435050.6	31025.0

**Precision Test****Pass****Radial**

Element Wavelength	Specification	Measured Value % RSD
As (188.980 nm)	≤ 2.60	0.81
Se (196.026 nm)	≤ 2.60	0.98
Zn (213.857 nm)	≤ 1.50	0.22
Pb (220.353 nm)	≤ 2.60	0.37
Mn (257.610 nm)	≤ 1.50	0.27
Al (396.152 nm)	≤ 1.50	0.25
Ba (493.408 nm)	≤ 1.50	0.53
K (766.491 nm)	≤ 1.50	0.15

**Axial**

Element Wavelength	Specification	Measured Value % RSD
As (188.980 nm)	≤ 1.50	0.81
Se (196.026 nm)	≤ 1.50	0.65
Zn (206.200 nm)	≤ 1.50	0.79
Zn (213.857 nm)	≤ 1.50	0.81
Cd (214.439 nm)	≤ 1.50	0.35
Pb (220.353 nm)	≤ 1.50	0.33
Mn (257.610 nm)	≤ 1.50	1.02
Cr (267.716 nm)	≤ 1.50	0.32
Cu (324.754 nm)	≤ 1.50	0.51
Al (396.152 nm)	≤ 1.50	0.37
Ba (493.408 nm)	≤ 1.50	0.68
K (766.491 nm)	≤ 1.50	0.74

**Report Summary**

Instrument Model	Agilent 5100/5110 VDV ICP-OES
Instrument ID	G8011A/G8015A
Instrument Serial Number	MY18030001
Software Version	7.3.1.9507
Firmware Version	3442
Tested By	Post Test_PM_Kanyakorn S.
Test Completed On	11/4/2024 11:30:15 AM

**Result Summary**

Subsystem Communications Test	Pass
Air Flow Test	Pass
Water Flow Test	Pass
Gas Flows Test	Pass
RF Generator Test	Pass
Camera Test	Pass
Optics Test	Skipped
Advanced Valve System Test	Skipped
Resolution Test	Skipped
Sensitivity Test	Skipped
Precision Test	Skipped

Subsystem Communications Test	Pass
-------------------------------	------

Air Flow Test	Pass
---------------	------

30% Air Flow (relative speed)	75% Air Flow (relative speed)
15.00	19.00

Water Flow Test	Pass
-----------------	------

RF Water Flow(L/min)	Camera Water Flow (L/min)	Water Inlet Temperature (°C)
1.30	0.81	20.55

**Gas Flows Test****Pass**

Nebulizer Target Flow	Actual Flow	Back Pressure	Auxiliary Target Flow	Actual Flow	Back Pressure
0.70	0.70	154.65	2.00	2.00	110.92
Makeup Target Flow	Actual Flow	Back Pressure	Plasma Target Flow	Actual Flow	Back Pressure
2.00	2.00	115.38	18.00	17.97	21.48

**RF Generator Test****Pass**

RF Power Supply Test	Passed
RF Power Supply (V)	128.554
RF Oscillator Test	Passed
RF Oscillator Frequency (MHz)	25.834
Work Coil Current (A)	44.660
RF Power Supply Current (A)	1.999

**Camera Test****Pass**

	Integration Time (ms)	Standard Deviation	Status
Electronic Offset Test	1000	5.228	Passed
Dark Current Test	6000	1.168	Passed
Array Test	5	0.024	Passed
Linearity Test		0.118	Passed



### Report Summary

Instrument Model	Agilent 5100/5110 VDV ICP-OES
Instrument ID	G8011A/G8015A
Instrument Serial Number	MY18030001
Software Version	7.3.1.9507
Firmware Version	3442
Tested By	change mirror
Test Completed On	11/6/2024 10:35:26 AM

### Result Summary

Subsystem Communications Test	Skipped
Air Flow Test	Skipped
Water Flow Test	Skipped
Gas Flows Test	Skipped
RF Generator Test	Skipped
Camera Test	Skipped
Optics Test	Skipped
Advanced Valve System Test	Skipped
Resolution Test	Pass
Sensitivity Test	Pass
Precision Test	Pass

**Resolution Test****Pass**

Element Wavelength	Specification	Width
N (174.213 nm)	≤ 9.40	6.79
As (188.980 nm)	≤ 8.20	5.80
C (193.027 nm)	≤ 11.50	8.15
Mo (202.032 nm)	≤ 8.20	5.90
Cr (206.158 nm)	≤ 13.40	8.85
Zn (213.857 nm)	≤ 8.70	6.77
Pb (220.353 nm)	≤ 9.50	6.61
Co (228.615 nm)	≤ 17.20	11.79
Ba (230.424 nm)	≤ 9.40	7.25
Mn (257.610 nm)	≤ 13.30	9.47
Mn (260.568 nm)	≤ 20.30	14.50
Cr (267.716 nm)	≤ 11.00	7.91
Cu (324.754 nm)	≤ 25.00	18.72
Cu (327.395 nm)	≤ 14.20	11.09
Sr (338.071 nm)	≤ 33.50	25.39
Ba (455.403 nm)	≤ 44.00	33.09
Sr (460.733 nm)	≤ 36.00	18.54
Ba (493.408 nm)	≤ 36.00	25.74
Ba (614.171 nm)	≤ 42.00	25.23
Ar (675.283 nm)	≤ 74.00	58.92
K (766.491 nm)	≤ 80.00	63.16

**Sensitivity Test****Pass****Radial**

Element Wavelength	Specification	Method	Ratio	Standard	Blank
As (188.980 nm)	≥ 46.0	SRBR	110.5	868.9	54.3
Se (196.026 nm)	≥ 41.0	SRBR	88.3	934.7	91.3
Zn (213.857 nm)	≥ 1421.0	SRBR	3535.4	44017.7	153.9
Pb (220.353 nm)	≥ 46.0	SRBR	184.5	2492.3	159.8
Mn (257.610 nm)	≥ 3518.0	SRBR	11099.6	249595.3	503.6
Al (396.152 nm)	≥ 3.4	SBR	8.7	50274.4	5172.0
Ba (493.408 nm)	≥ 34.0	SBR	124.5	1903164.1	15166.0
K (766.491 nm)	≥ 1.8	SBR	6.9	110041.4	13991.2

**Axial**

Element Wavelength	Specification	Method	Ratio	Standard	Blank
As (188.980 nm)	≥ 208.0	SRBR	253.3	3744.3	196.3
Se (196.026 nm)	≥ 159.0	SRBR	206.7	4199.7	347.2
Zn (206.200 nm)	≥ 234.0	SRBR	923.0	12282.3	172.1
Zn (213.857 nm)	≥ 1743.0	SRBR	6398.3	157551.5	601.7
Cd (214.439 nm)	≥ 4227.0	SRBR	5069.2	99873.7	385.2
Pb (220.353 nm)	≥ 320.0	SRBR	389.0	10641.1	658.6
Mn (257.610 nm)	≥ 10625.0	SRBR	21190.4	985528.7	2153.6
Cr (267.716 nm)	≥ 1048.0	SRBR	3054.1	131797.6	1811.5
Cu (324.754 nm)	≥ 19.0	SBR	36.3	301401.4	8082.9
Al (396.152 nm)	≥ 6.0	SBR	10.8	228359.5	19280.5
Ba (493.408 nm)	≥ 60.0	SBR	106.5	6460421.5	60122.8
K (766.491 nm)	≥ 24.0	SBR	30.2	1639840.6	52562.1

**Precision Test****Pass****Radial**

Element Wavelength	Specification	Measured Value % RSD
As (188.980 nm)	$\leq 2.60$	1.56
Se (196.026 nm)	$\leq 2.60$	1.16
Zn (213.857 nm)	$\leq 1.50$	0.50
Pb (220.353 nm)	$\leq 2.60$	0.74
Mn (257.610 nm)	$\leq 1.50$	0.63
Al (396.152 nm)	$\leq 1.50$	0.54
Ba (493.408 nm)	$\leq 1.50$	0.78
K (766.491 nm)	$\leq 1.50$	0.44

**Axial**

Element Wavelength	Specification	Measured Value % RSD
As (188.980 nm)	$\leq 1.50$	0.82
Se (196.026 nm)	$\leq 1.50$	0.82
Zn (206.200 nm)	$\leq 1.50$	0.35
Zn (213.857 nm)	$\leq 1.50$	0.34
Cd (214.439 nm)	$\leq 1.50$	0.44
Pb (220.353 nm)	$\leq 1.50$	0.48
Mn (257.610 nm)	$\leq 1.50$	0.83
Cr (267.716 nm)	$\leq 1.50$	0.53
Cu (324.754 nm)	$\leq 1.50$	0.69
Al (396.152 nm)	$\leq 1.50$	0.56
Ba (493.408 nm)	$\leq 1.50$	1.29
K (766.491 nm)	$\leq 1.50$	0.74

List of Instruments Certification for Air & Noise Quality Analysis

No.	Instrument/Equipment	Parameter	Manufacturer	Model/Serial No.	Calibrator	Certification No.	Date of Calibration	Due date of Calibration	Remark
Stack									
1	Pre-Test Console	Total Suspended Particulate	Apex Instruments, USA.	XC-572-V 1701019	Envi Equipment Service Co., Ltd.	E24-060048	18 Jun 24	17 Jun 25	-
2	Flue gas Analyzer	Sulphur Dioxide Oxide of Nitrogen as Nitrogen Dioxide	Testo	Testo 350 60899698/701	Entech Industrial Sultion Co., Ltd.	G 670083	8 Feb 24	7 Feb 25	-

List of Instruments Certification for Air & Noise Quality Analysis

No.	Instrument/Equipment	Parameter	Manufacturer	Model/Serial No.	Calibrator	Certification No.	Date of Calibration	Due date of Calibration	Remark
Ambient									
1	Orifice Transfer Standard Calibrator	Total Suspended Particulate (TSP) Particulate Matter < 10 µm (PM <sub>10</sub> )	Andersen Instruments, Inc.	G25A 1901	Jiranatee Associates Co., Ltd.	COF-002-66	14 Jul 23	13 Jul 25	-
2	U-Tube Manometer	Total Suspended Particulate (TSP) Particulate Matter < 10 µm (PM <sub>10</sub> )	Dwyer	1221-36-W/M -	Technology Promotion Association (Thailand-Japan)	24P1251	11 Apr 24	10 Apr 25	-
3	Aneroid Barometer	Total Suspended Particulate (TSP) Particulate Matter < 10 µm (PM <sub>10</sub> )	Barigo, Germany	-	Technology Promotion Association (Thailand-Japan)	24P1369	22 Apr 24	21 Apr 25	-
4	Dial Thermo-Hygrometer	Total Suspended Particulate (TSP) Particulate Matter < 10 µm (PM <sub>10</sub> )	Barigo, Germany	-	Technology Promotion Association (Thailand-Japan)	24H753	10 Apr 24	9 Apr 25	-
5	Nitrogen Dioxide Analyzer	Nitrogen Dioxide	Thermo Scientific	42i CM08130002	UAE Consultant Co.,Ltd.	17092024	17 Sep 24	16 Sep 25	-
6	Nitrogen Dioxide Analyzer	Nitrogen Dioxide	Thermo Scientific	42i CM19050148	UAE Consultant Co.,Ltd.	20092024	20 Sep 24	19 Sep 25	-
7	Nitrogen Dioxide Analyzer	Nitrogen Dioxide	Thermo Scientific	42i CM19050149	UAE Consultant Co.,Ltd.	17092024	17 Sep 24	16 Sep 25	-
8	Standard Gases (Mixture)	Nitrogen Dioxide	Airgas	EB0162121 2016PSIG	Airgas an Air Liquide company	E05NI91E15A0014	6 Jun 23	6 Jun 31	-
9	Sulphur Dioxide Analyzer	Sulphur Dioxide	Thermo Scientific	43i CM22387061	UAE Consultant Co.,Ltd.	06092024	6 Sep 24	5 Sep 25	-
10	Sulphur Dioxide Analyzer	Sulphur Dioxide	Thermo Scientific	43i CM22387063	UAE Consultant Co.,Ltd.	19062024	19 Jun 24	18 Jun 25	-
11	Sulphur Dioxide Analyzer	Sulphur Dioxide	Thermo Scientific	43i CM22387067	UAE Consultant Co.,Ltd.	15052024	15 May 24	14 May 25	-
12	Standard Gases (Mixture)	Nitrogen Dioxide	Airgas	EB0162121 2016PSIG	Airgas an Air Liquide company	E05NI91E15A0014	6 Jun 23	6 Jun 31	-
13	Sound Level Calibrator (Acoustic Calibrator)	Calibrate Sound Level Meter	Svantek	SV36 107224	Innovative Instrument Co.,Ltd.	24-ACT-091	26 Jun 24	25 Jun 25	-



List of Instruments Certification for Air & Noise Quality Analysis

No.	Instrument/Equipment	Parameter	Manufacturer	Model/Serial No.	Calibrator	Certification No.	Date of Calibration	Due date of Calibration	Remark
Ambient									
14	Sound Level Meter	L <sub>Aeq</sub> 1 hours <sup>+</sup> L <sub>Aeq</sub> 24 hrs <sup>+</sup> L <sub>Amax</sub> <sup>+</sup> L <sub>A90</sub> <sup>+</sup>	Larson Davis	LxT2	Electrical And Electronics Institute Foundation For Industrial Development	CP20240292EA	6 Aug 24	5 Aug 25	-
				0005348					
15	Sound Level Meter	L <sub>Aeq</sub> 1 hours <sup>+</sup> L <sub>Aeq</sub> 24 hrs <sup>+</sup> L <sub>Amax</sub> <sup>+</sup> L <sub>A90</sub> <sup>+</sup>	Larson Davis	LxT2	Innovative Instrument Co.,Ltd.	24-SLM-237	10 Jul 24	9 Jul 25	-
				0005393					
16	Sound Level Meter	L <sub>Aeq</sub> 1 hours <sup>+</sup> L <sub>Aeq</sub> 24 hrs <sup>+</sup> L <sub>Amax</sub> <sup>+</sup> L <sub>A90</sub> <sup>+</sup>	Larson Davis	LxT2	Electrical And Electronics Institute Foundation For Industrial Development	CP20240291EA	5 Aug 24	4 Aug 25	-
				0005396					

List of Instruments Certification for Air & Noise Quality Analysis

No.	Instrument/Equipment	Parameter	Manufacturer	Model/Serial No.	Calibrator	Certification No.	Date of Calibration	Due date of Calibration	Remark
Workplace									
1	Primary Flow Calibrator	Calibrate personal pump	TSI,Inc	4146 41462327003	Innovative Instrument Co., Ltd.	24-AFM-158	19 Aug 24	18 Aug 25	-
2	Air Sampling Pump	Ethyl Alcohol Total Dust Respirable Dust TVOCs	Sensidyne	GilAir Plus 20230610196	Innovative Instrument Co., Ltd.	24-ASP-127	27 Aug 24	26 Aug 25	-
3	Air Sampling Pump	Ethyl Alcohol Total Dust Respirable Dust TVOCs	Sensidyne	GilAir Plus 20230410024	Innovative Instrument Co., Ltd.	24-ASP-048	8 May 24	7 May 25	-
4	Air Sampling Pump	Ethyl Alcohol Total Dust Respirable Dust TVOCs	Sensidyne	GilAir Plus 20230410025	Innovative Instrument Co., Ltd.	24-ASP-041	6 May 24	5 May 25	-
5	Air Sampling Pump	Ethyl Alcohol Total Dust Respirable Dust TVOCs	Sensidyne	GilAir Plus 20230410027	Innovative Instrument Co., Ltd.	24-ASP-040	3 May 24	2 May 25	-
6	Air Sampling Pump	Ethyl Alcohol Total Dust Respirable Dust TVOCs	Sensidyne	GilAir Plus 20230410021	Innovative Instrument Co., Ltd.	24-ASP-045	7 May 24	6 May 25	-
7	Air Sampling Pump	Ethyl Alcohol Total Dust Respirable Dust TVOCs	Sensidyne	GilAir Plus 20230610198	Innovative Instrument Co., Ltd.	24-ASP-122	26 Aug 24	25 Aug 25	-
8	Air Sampling Pump	Ethyl Alcohol Total Dust Respirable Dust TVOCs	Sensidyne	GilAir Plus 20230610205	Innovative Instrument Co., Ltd.	24-ASP-125	27 Aug 24	26 Aug 25	-
9	Aneroid Barometer	Ethyl Alcohol Total Dust Respirable Dust TVOCs							
9	Aneroid Barometer	Ethyl Alcohol Total Dust Respirable Dust TVOCs	Barigo, Germany	-	Technology Promotion Association (Thailand-Japan)	24P1370	22 Apr 24	21 Apr 25	-
10	Digital Thermo - Hygrometer	Temperature Humidity Respirable Dust TVOCs	Digicon	TH-02 395034172	Technology Promotion Association (Thailand-Japan)	24H717	10 Apr 24	9 Apr 25	-
11	Gas Detector	TVOCs	RAE Systems, Inc.	MiniRAE 3000+ 592-928075	Executive Trading Limited	RA 187/24	7 Aug 24	6 Aug 25	-
12	Sound Level Calibrator (Acoustic Calibrator)	Calibrate Sound Level Meter	Larson Davis	CAL150 6306	Innovative Instrument Co.,Ltd.	24-ACT-067	17 May 24	16 May 25	-
13	Sound Level Meter	L <sub>Aeq</sub> 8 hrs <sup>+</sup> L <sub>Amax</sub>	Rion, Japan	NL-42 00709670	Sithiporn Associates Co., Ltd.	ACL24061	18 Jan 24	17 Jan 25	-
14	Sound Level Meter	L <sub>Aeq</sub> 8 hrs <sup>+</sup> L <sub>Amax</sub>	Rion, Japan	NL-42 00609500	Sithiporn Associates Co., Ltd.	ACL24058	18 Jan 24	17 Jan 25	-
15	Thermal Environment Monitor	Heat Meter	TSI QUEST	QuesTemp 34 TEX040015	Innovative Instrument Co.,Ltd.	24-TPM-313	9 Jul 24	8 Jul 25	-
16	Thermal Environment Monitor	Heat Meter	Quest Technologies, Inc	QuesTemp 34 TEK120020	Innovative Instrument Co.,Ltd.	24-TPM-371	15 Aug 24	14 Aug 25	-

List of Instruments Certification for Water Quality Analysis

No.	Instrument/Equipment	Parameter	Manufacturer	Model/Serial No.	Calibrator	Certification No.	Date of Calibration	Due date of Calibration	Remark
Water									
1	pH Meter	pH	Horiba	LAQUA-PH210 HA0D0078	Technology Promotion Association (Thailand-Japan)	24CH239	20 Feb 24	19 Feb 25	-

List of Instruments Certification for Air & Noise Quality Analysis

No.	Instrument/Equipment	Parameter	Manufacturer	Model/Serial No.	Calibrator	Certification No.	Date of Calibration	Due date of Calibration	Remark
Workplace									
1	Sound Level Calibrator (Acoustic Calibrator)	Calibrate Sound Level Meter	Svantek	SV36 107224	Innovative Instrument Co.,Ltd.	24-ACT-091	26 Jun 24	25 Jun 25	-
2	Sound Level Meter	$L_{Aeq\ 12\ hrs}$ , $L_{Aeq\ 8\ hrs}$ , $L_{Amax}$	Rion, Japan	NL-42 00709655	Sithiporn Associates Co., Ltd.	ACL24060	18 Jan 24	17 Jan 25	-
3	Sound Level Meter	$L_{Aeq\ 12\ hrs}$ , $L_{Aeq\ 8\ hrs}$ , $L_{Amax}$	Rion, Japan	NL-42 01010782	Sithiporn Associates Co., Ltd.	ACL24166	6 Jun 24	5 Jun 25	-
4	Sound Level Meter	$L_{Aeq\ 12\ hrs}$ , $L_{Aeq\ 8\ hrs}$ , $L_{Amax}$	Rion, Japan	NL-42 00408981	Sithiporn Associates Co., Ltd.	ACL24098	29 Jan 24	28 Jan 25	-
5	Sound Level Meter	$L_{Aeq\ 12\ hrs}$ , $L_{Aeq\ 8\ hrs}$ , $L_{Amax}$	Rion, Japan	NL-42 00609500	Sithiporn Associates Co., Ltd.	ACL24058	18 Jan 24	17 Jan 25	-
6	Sound Level Meter	$L_{Aeq\ 12\ hrs}$ , $L_{Aeq\ 8\ hrs}$ , $L_{Amax}$	Rion, Japan	NL-42 00321441	Sithiporn Associates Co., Ltd.	ACL24156	30 May 24	29 May 25	-
7	Sound Level Meter	$L_{Aeq\ 12\ hrs}$ , $L_{Aeq\ 8\ hrs}$ , $L_{Amax}$	Rion, Japan	NL-42 00409175	Sithiporn Associates Co., Ltd.	ACL24055	18 Jan 24	17 Jan 25	-
8	Sound Level Meter	$L_{Aeq\ 12\ hrs}$ , $L_{Aeq\ 8\ hrs}$ , $L_{Amax}$	Rion, Japan	NL-42 00709651	Sithiporn Associates Co., Ltd.	ACL24059	18 Jan 24	17 Jan 25	-
9	Sound Level Calibrator (Acoustic Calibrator)	Calibrate Sound Level Meter	01dB	CAL31 82795	Innovative Instrument Co.,Ltd.	24-ACT-065	17 May 24	16 May 25	-
10	Sound Level Meter	$L_{Aeq\ 12\ hrs}$ , $L_{Aeq\ 8\ hrs}$ , $L_{Amax}$	Rion, Japan	NL-42 00709656	Sithiporn Associates Co., Ltd.	ACL24155	30 May 24	29 May 25	-
11	Sound Level Meter	$L_{Aeq\ 12\ hrs}$ , $L_{Aeq\ 8\ hrs}$ , $L_{Amax}$	Rion, Japan	NL-42 00408981	Sithiporn Associates Co., Ltd.	ACL24098	29 Jan 24	28 Jan 25	-
12	Sound Level Meter	$L_{Aeq\ 12\ hrs}$ , $L_{Aeq\ 8\ hrs}$ , $L_{Amax}$	Rion, Japan	NL-62 00511774	Sithiporn Associates Co., Ltd.	ACL24159	4 Jun 24	3 Jun 25	-
13	Sound Level Meter	$L_{Aeq\ 12\ hrs}$ , $L_{Aeq\ 8\ hrs}$ , $L_{Amax}$	Rion, Japan	NL-42 00409109	Sithiporn Associates Co., Ltd.	ACL24054	18 Jan 24	17 Jan 25	-

List of Instruments Certification for Air & Noise Quality Analysis

No.	Instrument/Equipment	Parameter	Manufacturer	Model/Serial No.	Calibrator	Certification No.	Date of Calibration	Due date of Calibration	Remark
Workplace									
14	Sound Level Meter	L <sub>Aeq</sub> 12 hrs <sup>a</sup> L <sub>Aeq</sub> 8 hrs <sup>a</sup> L <sub>Amax</sub>	Rion, Japan	NL-42 01010778	Sithiporn Associates Co., Ltd.	ACL24157	30 May 24	29 May 25	-
15	Sound Level Meter	L <sub>Aeq</sub> 12 hrs <sup>a</sup> L <sub>Aeq</sub> 8 hrs <sup>a</sup> L <sub>Amax</sub>	Rion, Japan	NL-62 00881367	Sithiporn Associates Co., Ltd.	ACL24065	18 Jan 24	17 Jan 25	-
16	Sound Level Meter	L <sub>Aeq</sub> 12 hrs <sup>a</sup> L <sub>Aeq</sub> 8 hrs <sup>a</sup> L <sub>Amax</sub>	Rion, Japan	NL-42 00558212	Sithiporn Associates Co., Ltd.	ACL24100	29 Jan 24	28 Jan 25	-
17	Primary Flow Calibrator	Calibrate personal pump	TSI,Inc	4146 41462327002	Innovative Instrument Co., Ltd.	24-AFM-156	19 Aug 24	18 Aug 25	-
18	Air Sampling Pump	Benzene Toluene Xylene	Sensidyne	GiAir 5 20180102018	Innovative Instrument Co., Ltd.	24-ASP-075	14 Jun 24	13 Jun 25	-
19	Air Sampling Pump	Benzene Toluene Xylene	Sensidyne	GiAir 5 20150602023	Calibration Laboratory Co.Ltd	Q24050344	17 May 24	16 May 25	-
20	Air Sampling Pump	Benzene Toluene Xylene	Sensidyne	GiAir 5 20220301020	Innovative Instrument Co., Ltd.	24-ASP-100	28 Jun 24	27 Jun 25	-
21	Air Sampling Pump	Benzene Toluene Xylene	Sensidyne	GiAir 5 20170701011	Calibration Laboratory Co.Ltd	Q24050341	17 May 24	16 May 25	-
22	Air Sampling Pump	Benzene Toluene Xylene	Sensidyne	GiAir 5 20150601001	Calibration Laboratory Co.Ltd	Q24050342	17 May 24	16 May 25	-
23	Air Sampling Pump	Benzene Toluene Xylene	Sensidyne	GiAir 5 20120301017	Calibration Laboratory Co.Ltd	Q24050345	17 May 24	16 May 25	-

List of Instruments Certification for Air & Noise Quality Analysis

No.	Instrument/Equipment	Parameter	Manufacturer	Model/Serial No.	Calibrator	Certification No.	Date of Calibration	Due date of Calibration	Remark
Workplace									
24	Aneroid Barometer	Benzene Toluene Xylene	Barigo, Germany	-	Technology Promotion Association (Thailand-Japan)	24P1145	9 Apr 24	8 Apr 25	-
25	Digital Thermo - Hygrometer	Benzene Toluene Xylene	Digicon	TH-02 395034173	Technology Promotion Association (Thailand-Japan)	24H716	10 Apr 24	9 Apr 25	-

**Envi Equipment Service Co., Ltd.**

110/254 Moo 3, Tumbon Bang Rak Phatthana, Amphur Bang Bua Thong, Nonthaburi 11110

Tel. 098 362 9152, 089 478 7885

E-mail: sales@envi-ees.com

Certificate No.: E24-060048

Page.: 1 of 6

**CERTIFICATE OF CALIBRATION**

**Customer** : United Analyst and Engineering Consultant Co., Ltd.

**Address** : 81 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260

**Description of Equipment** : Console meter

**Manufacturer** : Apex Instrument

**Model Number** : XC-572-V

**Serial Number** : 1701019

**ID./Control No.** : UAE.EFM 013/2560

**Environment Conditions** : Temperature (25 ± 2) °C  
: Humidity (50 ± 15) % RH

**Cal. Date** : 18/06/2024

**Issue Date** : 18/06/2024

**Calibration Method or Calibration Procedure Used**

US EPA Method (United State Environmental Protection Agency)

This certificate is traceable to national standard, which realize the units of measurement according to the International System of Units (IS).

**Result of Calibration**

This certificate may not be reproduced other than in full except with prior Written approval of the Technical Manager, Envi Equipment Service Company Limited.

These reported uncertainties of measurement are expanded by a coverage factor of k=2, providing a 95% confidence level

Calibrated by : Mr. Sanya Sangnil

Approved by :



(Mr. Mana Fueklud)

Technical Manger

**เอกสารไม่ควบคุม**

**METHOD 5 CONSOLE CALIBRATION**  
**USING REFERENCE WET GAS METER W-NK-2.5-B-Z No.547425**  
**5-POINT METRIC UNIT**

Meter Console Information		Calibration Conditions				Factors/Conversions		
Console Model Number	XC-572-V	Date	Time	18/06/2024	10:00 AM	Std Temp	293	K
Console Serial Number	1701019	Calibration Reference No.		SER24-060018		Std Press	760	mm Hg
DGM Model Number	SK25EX	Barometric Pressure		755.91	mmHg	K <sub>1</sub>	0.386	
DGM Serial Number	00002028	Calibration Meter Gamma		1.001		Console Leak Check		PASS

Calibration Data									
Run Time	Metering Console					Calibration Meter			
Elapsed	DGM Orifice DH	Volume Initial	Volume Final	Outlet Temp Initial	Outlet Temp Final	Volume Initial	Volume Final	Outlet Temp Initial	Outlet Temp Final
(Q)	(P <sub>m</sub> )	(V <sub>mi</sub> )	(V <sub>mf</sub> )	(t <sub>mi</sub> )	(t <sub>mf</sub> )	(V <sub>wi</sub> )	(V <sub>wf</sub> )	(t <sub>wi</sub> )	(t <sub>wf</sub> )
min	mm H <sub>2</sub> O	m <sup>3</sup>	m <sup>3</sup>	°C	°C	m <sup>3</sup>	m <sup>3</sup>	°C	°C
11.82	13.0	2802.112	2802.252	32	32	222.03382	222.17160	29	29
11.85	13.0	2802.252	2802.392	32	32	222.17160	222.30948	29	29
8.42	26.0	2802.399	2802.539	32	32	222.31644	222.45472	29	29
8.43	26.0	2802.539	2802.679	32	32	222.45472	222.59264	29	29
13.80	40.0	2802.686	2802.966	32	32	222.59970	222.87558	28	28
13.78	40.0	2802.966	2803.246	32	32	222.87558	223.15024	27	27
10.32	70.0	2803.261	2803.541	33	33	223.16476	223.43840	27	27
10.33	70.0	2803.541	2803.821	33	33	223.43840	223.71148	27	27
9.00	90.0	2803.835	2804.115	33	33	223.72450	223.99668	27	27
9.00	90.0	2804.115	2804.395	33	33	223.99668	224.26896	27	27



**เอกสารไม่ควบคุม**



**METHOD 5 CONSOLE CALIBRATION  
USING REFERENCE WET GAS METER W-NK-2.5-B-Z No.547425  
5-POINT METRIC UNIT**

Meter Console Information		Calibration Conditions				Factors/Conversions		
Console Model Number	XC-572-V	Date	Time	18/06/2024	10:00 AM	Std Temp	293	K
Console Serial Number	1701019	Calibration Reference No.		SER24-060018		Std Press	760	mm Hg
DGM Model Number	SK25EX	Barometric Pressure		755.91		K <sub>1</sub>	0.386	
DGM Serial Number	00002028	Calibration Meter Gamma		1.001		Console Leak Check		PASS

Calibration Data								
Results								
Standardized Data				Dry Gas Meter				
Dry Gas Meter		Calibration Meter		Calibration Factor		Flowrate		
(V <sub>m(std)</sub> )	(Q <sub>m(std)</sub> )	(V <sub>w(std)</sub> )	(Q <sub>w(std)</sub> )	Value	Variation	Std & Corr	.0212 m <sup>3</sup> <sub>std</sub> /min	Variation
m <sup>3</sup>	m <sup>3</sup> /min	m <sup>3</sup>	m <sup>3</sup> /min	(Y)	(ΔY)	(Q <sub>m(std)</sub> )(corr))	(ΔH <sub>@</sub> )	(ΔH <sub>@</sub> )
						m <sup>3</sup> /min	mm H <sub>2</sub> O	
0.135	0.011	0.133	0.011	0.984	0.007	0.011	44.706	-1.370
0.135	0.011	0.133	0.011	0.985	0.008	0.011	44.893	-1.182
0.135	0.016	0.134	0.016	0.986	0.009	0.016	45.148	-0.928
0.135	0.016	0.133	0.016	0.984	0.007	0.016	45.564	-0.512
0.272	0.020	0.267	0.019	0.982	0.005	0.019	46.883	0.808
0.273	0.020	0.267	0.019	0.978	0.001	0.019	47.030	0.954
0.274	0.027	0.266	0.026	0.972	-0.005	0.026	46.723	0.648
0.274	0.027	0.266	0.026	0.970	-0.007	0.026	47.067	0.991
0.274	0.030	0.265	0.029	0.965	-0.012	0.029	46.388	0.313
0.274	0.030	0.265	0.029	0.965	-0.012	0.029	46.354	0.279
				0.977	Y Average		46.075	ΔH <sub>@</sub> Average

**Note:** For Calibration Factor Y, the ratio of the reading of the calibration meter to the dry gas meter, acceptable tolerance of individual values from the average is ±0.02.

For ΔH<sub>@</sub>, orifice pressure differential that equates to 0.75 cfm (0.0212 m<sup>3</sup>/min) at standard temperature and pressure, acceptable tolerance of individual values from the average is ±0.2 inches (5.1mm) to



**เอกสารไม่ควบคุม**

Meter Console Information	
Console Model Number	XC-572-V
Console Serial Number	1701019
DGM Model Number	SK25EX
DGM Serial Number	00002028


Calibration Conditions			
Date	Time	18/06/2024	10:00 AM
Calibration Reference No.	SER24-060018		
Barometric Pressure	755.91	mmHg	
Calibration Meter Gamma	1.001		

Factors/Conversions		
Std Temp	293	K
Std Press	760	mm Hg
K <sub>1</sub>	0.386	
Console Leak Check	PASS	

Calibration Date: 18-6-2024

Calibration Reference No: SER24-060018

Meter Gamma vs Flowrate

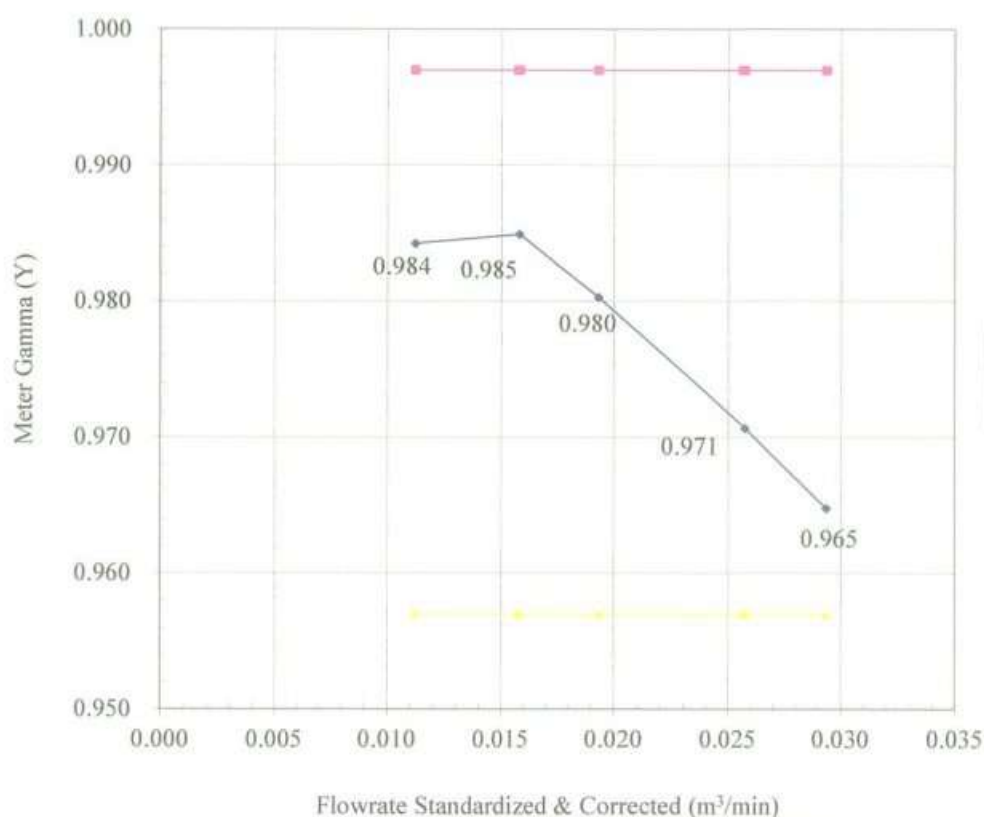

Console Serial: 1701019

Console Model: XC-572-V




เอกสารไม่ควบคุม

Meter Console Information		Calibration Conditions				Factors/Conversions		
Console Model Number	XC-572-V	Date	Time	18/06/2024	10:00 AM	Std Temp	293	K
Console Serial Number	1701019	Calibration Reference No.		SER24-060018		Std Press	760	mm Hg
DGM Model Number	SK25EX	Barometric Pressure		755.91	mmHg	K <sub>i</sub>	0.386	
DGM Serial Number	00002028	Calibration Meter Gamma		1.001		Console Leak Check		PASS

Calibration Date: 18-6-2024

Calibration Reference No: SER24-060018

**Meter Pressure vs Flowrate**

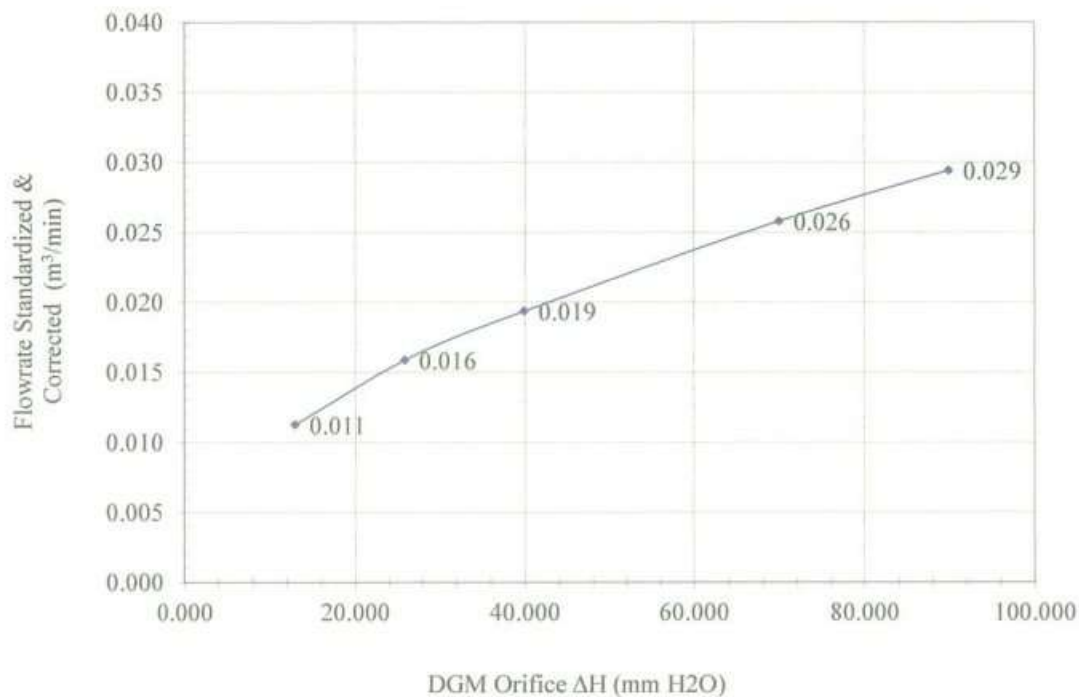

Console Serial: 1701019

Console Model: XC-572-V



เอกสารไม่ควบคุม



## THERMOCOUPLES SYSTEM CALIBRATION

Sampling System Equipment Information	
Console Model Number	XC-572-V
Console Serial Number	1701019
DGM Model Number	SK25EX
DGM Serial Number	00002028
Meter Box Model Number	JENCO 765 KF
Meter Box Serial Number	JC 19777

Calibration Conditions			
Date	Time	18/06/2024	00:20 PM
Calibration Reference No.	SER24-060018		
Reference Thermometer	DIGICON		
Serial Number	183169105		

Results											
Console Thermocouple Simulator											
Channel and test point	Meter Box Channel Temperature Reading ( °C )										
	-18.0	25.0	38.0	93.0	149.0	260.0	371.0	482.0	593.0	816.0	1038.0
Stack	-17.0	25.0	38.0	93.0	149.0	257.0	368.0	477.0	587.0	806.0	1024.0
Aux	-17.0	25.0	38.0	93.0	149.0						
Probe	-17.0	25.0	38.0	93.0	149.0						
Filter	-17.0	25.0	38.0	93.0	149.0						
Oven	-17.0	25.0	38.0	93.0	149.0						
Exit	-17.0	25.0	38.0								

### Tolerance Range

Stack      ± 1.50%      Absolute  
 Probe      ± 3.0 °C  
 Filter      ± 3.0 °C

Meter      ± 3.0 °C  
 Exit        ± 2.0 °C



เอกสารไม่ควบคุม

**Certificate No:** G 670083

**Date of issue :** 08-Feb-24

**Instrument description :** Flue Gas Analyzer  
**Instrument model :** Testo 350 New  
**Control unit serial no. :** 03099393/701  
**Instrument serial no. :** 60899698/701  
**ID no. or control no. :** UAE.EFM.008/2560  
**Manufacturer :** Testo SE & Co. KGaA  
**Probe description :** -  
**Probe model :** -  
**Probe serial no. :** -  
**Customer name :** UNITED ANALYST CONSULTANT CO.,LTD.  
**Customer address :** 81 SOI UDOMSUK41,SUKHUMVIT ROAD,BANGCHAK PRAKANONG BANGKOK 10260

**Total pages of certificate :** 2 Pages  
**Receiving no. :** L-240430  
**Receiving date. :** 05-Feb-24  
**Parameter of calibration :** Gas Calibration(Oxygen 2.50,10.04,21.02 %vol, Carbon Monoxide 80.14,302,1003 ppm, Nitrogen Dioxide 30.34,81.32, 201.9 ppm, Nitric Oxide 30.01, 151.5, 322.5 ppm, Sulphur Dioxide 50.36, 100.8, 600.8 ppm)  
**Condition of UUC. :** Used  
**Ambient condition :** All of the Measurment ware caried out the stabilized labotary  
 Temperature : 23 ± 5 °C  
 Humidity : 55 ± 15 %RH  
**Calibration place :** 17/121 Soi Ngamwongwan 47 Yaek 48, Toongsonghong, Laksi, Bangkok 10210  
**Calibration procedure no. :** This instrument was calibrated by comparison with Standard gas mixture according to calibration Work Instruction no. WI-CL-28-C

*The calibration certificate expanded uncertainty of measurement is stated as the standard uncertainty of measurent Multiplied by coverage factor  $k=2$ , which for a normal distribution corresponds to a coverage probability of approximately 95%.*

*This certificate is applied only to item under test Environmental condition.*

*This Calibration Certificate may not be reporduced other than in full except with the permission of the issuing laboratory. Calibration certificates without signature and seal not valid and The results relate only to the items tested/calibrated.*

*This calibration certificate documents are tracebility to national standards, which realize measurement according to the International System of Units (SI).*

**Date of calibration :** 08-Feb-24



Mr. Kwanchai Khamdoun  
Calibration Technician



Mrs. Nongluck Wongsettee  
Technical Manager



Certificate No.: G 670083

### Standard References (Table 1)

Standard	Certificate No.	Vendor	Due date
Oxygen ( O <sub>2</sub> ) 2.50 % Vol	2412/23	Linde	27-Aug-27
Oxygen ( O <sub>2</sub> ) 10.04 % Vol	CG-0153-21	Nimt	18-Nov-26
Oxygen ( O <sub>2</sub> ) 21.02 % Vol	CG-0041-22	Nimt	10-Feb-27
Carbon monoxide ( CO ) 80.14 ppm	CG-0040-22	Nimt	14-Feb-27
Carbon monoxide ( CO ) 302 ppm	1915/23	Linde	16-Jun-25
Carbon monoxide ( CO ) 1003 ppm	2584/23	Linde	10-Sep-25
Nitrogen Dioxide ( NO <sub>2</sub> ) 30.34 ppm	2703/22	Linde	22-Aug-24
Nitrogen Dioxide ( NO <sub>2</sub> ) 81.32 ppm	3546/23	Linde	14-Jan-26
Nitrogen Dioxide ( NO <sub>2</sub> ) 201.9 ppm	1975/23	Linde	17-Jul-25
Nitric Oxide ( NO ) 30.01 ppm	CG-0014-23	Nimt	19-Feb-25
Nitric Oxide ( NO ) 151.5 ppm	0161/23	Linde	22-Jan-25
Nitric Oxide ( NO ) 322.5 ppm	1974/23	Linde	17-Jul-25
Sulphur Dioxide ( SO <sub>2</sub> ) 50.36 ppm	2004/23	Linde	17-Jul-25
Sulphur Dioxide ( SO <sub>2</sub> ) 100.8 ppm	3507/22	Linde	09-Nov-24
Sulphur Dioxide ( SO <sub>2</sub> ) 600.8 ppm	2003/23	Linde	17-Jul-25

### Measured room conditions

Temperature : 23.5 °C Humidity : 64.1 %RH Pressure : 1011.7 mbar

### Calibration conditions

Gas Temperature : 23 °C Flow rate : 1,200 ml/min Gas pressure : 1016.4 mbar

### Calibration Results (Without adjustment) (Table 2)

Parameter of Standard	Standard Values	Mean of UUC	Error	Uncertainty (±)
O <sub>2</sub> (%Vol)	2.50	2.57	0.07	0.15
O <sub>2</sub> (%Vol)	10.04	10.09	0.05	0.20
O <sub>2</sub> (%Vol)	21.02	21.08	0.06	0.30
CO (ppm)	80.14	81	0.86	3.0
CO (ppm)	302	302	0	6.0
CO (ppm)	1003	1002	-1	12
NO <sub>2</sub> (ppm)	30.34	30.2	0.14	8.0
NO <sub>2</sub> (ppm)	81.32	82.4	1.08	8.0
NO <sub>2</sub> (ppm)	201.9	202.8	0.9	12
NO (ppm)	30.01	29	-1.01	8.0
NO (ppm)	151.5	150	-1.5	8.0
NO (ppm)	322.5	320	-2.5	12
SO <sub>2</sub> (ppm)	50.36	49	-1.36	6.0
SO <sub>2</sub> (ppm)	100.8	100	-0.8	6.0
SO <sub>2</sub> (ppm)	600.8	599	-1.8	13

Remark : 1 cmol/mol = 1 %vol. 1 µmol/mol = 1 ppm.

## End of Report



JIRANATEE ASSOCIATES CO.,LTD.

Jiranatee Associates Co.,Ltd  
63/14-15, 67/35-36  
Petchkasem 7,7/1, Rd. Watthapra, Bangkokyai,  
Bangkok 10600 (Thailand)  
Tel: +6608680812  
Mobile: +66863999453  
E-mail: jnac-calibration@jiranatee.com  
Web site: www.jiranatee.com

Accredited calibration laboratory  
ISO/IEC 17025:2017  
NSC-TISI-TIS 17025  
CALIBRATION 0367

Flow measurement laboratory  
Calibration services department.



## CERTIFICATE OF CALIBRATION

Certificate No. : COF-002-66

Page 1 of 2 Pages

**MEASUREMENT ITEM** : Top Load Orifice  
**MANUFACTURER** : Andersen Instruments  
**MODEL/TYPE** : G25A  
**SERIAL NUMBER** : 1901  
**ID NUMBER** : UAE.ANV.051/2547  
**CONDITION AS-RECEIVED** : Used Item  
**CUSTOMER** : United Analyst and Engineering Consultant Co., Ltd.  
81 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong,  
Bangkok 10260

**RECEIVED DATE** : 07 Jul 2023  
**MEASUREMENT DATE** : 14 Jul 2023  
**ISSUE DATE** : 18 Jul 2023

### ENVIRONMENTAL CONDITIONS:

Ambient condition in the laboratory are as follow:

Temperature	: $23.0 \pm 3.0$	°C
Relative Humidity	: $55.0 \pm 15.0$	%RH
Atmospheric Pressure	: $1010 \pm 10$	hPa

### CALIBRATION CONDITION:

Preconditioning : 24 hours at ambient conditions.  
Measurement Condition : The average values during measurement are 23.9 °C and 54.5%RH.

**NOTED:** The certificate is valid only to the item calibrated on date and place of calibration.

### TABULATION OF RESULTS:

The table on next page give the measured values.

### Calibration procedure:

The Orifice gas flow device was calibrated against Standard Rotary Displacement Meter (Roots Meter) Model G65/IMC/W2-dp. The WI-CL-004 was used as a calibration guideline.

### Traceability:

This certificate provides a traceability of The measurement to recognized the national standards, and to realization of the international system of units (SI) through the VSL (National Metrology Institute of Netherlands) via Certificate number: G2211901

### Uncertainty of Measurement:

The reported uncertainty of measurement is based on the standard uncertainty multiplied by a coverage factor  $k=2$ , Which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty has been determined in accordance with the GUM 'Evaluation of measurement data - Guide to the expression of uncertainty in measurement'

### Calibrated by:

- ☐ Mr. Sorawit Thachalad  
☒ Miss Jittraporn Lertsomphol



### Approved signatory:

Mr. Parinya Booncharoen  
Calibration Department Manager

เอกสารไม่ควบคุม

**MEASUREMENT RESULTS:**

The Orifice gas flow device was calibrated by direct comparison method with the Standard Rotary Displacement Meter (Roots Meter). The Humid air was used as a medium in the system. The standard conditions are 25°C (298.15 K) and 760 mmHg for standard temperature and standard pressure respectively.

**Table 1:** The results of  $Q$  Standard calibration data

Plate	Flow rate $m^3/min$	Pressure [Pa] mmHg	Temperature [Ta] °C	Temperature [Tm] °C	$\Delta p_{meter}$ mmHg	$\Delta p_{Orifice}$ inH <sub>2</sub> O	$\gamma$	Standard Flow [ $Q_s$ ] $m^3/min$
1	0.701	754.115	23.87	23.10	55.600	1.626	1.273	0.648
2	0.997	754.083	23.80	23.23	61.350	3.236	1.795	0.914
3	1.121	754.005	23.81	23.20	41.923	4.338	2.079	1.057
4	1.172	754.004	23.72	23.16	30.933	4.891	2.208	1.122
5	1.410	753.994	23.76	23.18	29.415	7.159	2.671	1.352

Slope ( $m$ ): 1.98463  
 Intercept ( $b$ ): -0.01636  
 Correlation coefficient ( $r$ ): 0.99972  
 Uncertainty ( $k=2$ ): 0.015  $m^3/min$

**Table 2:** The results of  $Q$  actual calibration data

Plate	Flow rate $m^3/min$	Pressure [Pa] mmHg	Temperature [Ta] °C	Temperature [Tm] °C	$\Delta p_{meter}$ mmHg	$\Delta p_{Orifice}$ inH <sub>2</sub> O	$\gamma$	Standard Flow [ $Q_a$ ] $m^3/min$
1	0.701	754.115	23.87	23.10	55.600	1.626	0.800	0.651
2	0.997	754.083	23.80	23.23	61.350	3.236	1.129	0.917
3	1.121	754.005	23.81	23.20	41.923	4.338	1.307	1.061
4	1.172	754.004	23.72	23.16	30.933	4.891	1.388	1.126
5	1.410	753.994	23.76	23.18	29.415	7.159	1.679	1.357

Slope ( $m$ ): 1.24306  
 Intercept ( $b$ ): -0.01029  
 Correlation coefficient ( $r$ ): 0.99972  
 Uncertainty ( $k=2$ ): 0.015  $m^3/min$

\*\*\*End of Certificate of Calibration\*\*\*



เอกสารไม่ควบคุม





## Certificate of Calibration

Certificate No. : 24P1251

Page : 1 of 2

Equipment : U Tube Manometer

Manufacturer: Dwyer

Model : 1221-36-W/M

Serial No.: -

ID No.: UAE.EFM.077/2566

Condition As-Received: Used Item

Received Date: 03 April 2024

Calibration Date: 11 April 2024

Reference: 2404-0118WSC

Ambient Temperature: ( 23 ± 2 ) °C

Relative Humidity: ( 50 ± 15 ) %

Atmospheric Pressure: 1012 mbar

Submitted by: United Analyst and Engineering Consultant Co.,Ltd.

This certificate may not be reproduced other than in full,  
except with the prior written approval of the head of  
Corporate Services 3: Equipment Calibration and Testing Services.

81 Soi Udomsuk 41, Sukhumvit Road, Bangchak,  
Phrakhanong, Bangkok 10260

**Procedure used:** The calibration was conducted by direct comparison method against Pressure Measuring Instruments Standard according to calibration procedure CP-P04, using " DKD-R 6-1 ; Calibration of Pressure Gauges " as a guidelines.

### Condition of this result of calibration

1.Reference standards instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Certificate No.</u>	<u>Due Date</u>
1) Pressure Calibrator	PC106P	1189	MP-0176-23	12 Sep 2024

2.This result of calibration was made on requested at the point specified by customer.

3.Scale and conversion factor is 1 kPa = 4.0146293 inH<sub>2</sub>O

4.This instrument was used clean air as pressure media.

5.This instrument was calibrated by applied pressure to high-port (+) side and low-port (-) side open to atmospheric pressure.

6.This instrument was installed in vertical orientation and top of the pressure port was used as the reference level.

7.The certificate is valid only to the item calibrated on date and place of calibration.

8.This Certification is traceable to the International System of Unit maintained through:-

-National Institute of Metrology (Thailand), NSC-ONSC Accredited No. Calibration 0144

Calibrated by : Suksan Khankaew

Issue Date : 17 April 2024

Approved Signatory :

[ ] Phalinee Prabpaipal

[ ] Sura Suwannasri

[✓] Attapol Panurach

เอกสารไม่ควบคุม



Cert.No.: 24P1251

Page: 2 of 2

**Result of calibration:- Without adjustment**

**Range :** 0 inH<sub>2</sub>O to 36 inH<sub>2</sub>O

**Function:- Pressure Measurement**

**Scale Interval :** 0.1 inH<sub>2</sub>O ( The Second Estimate )

**Increasing Pressure**

UUC Indication				
Applied Pressure	High-port side	Low-port side	$\Delta P$	Error
0.00	0.00	0.00	0.00	0.00
2.00	1.00	-1.00	2.00	0.00
4.00	2.00	-2.00	4.00	0.00
6.00	3.00	-3.00	6.00	0.00
8.00	4.00	-4.00	8.00	0.00
10.00	5.00	-5.00	10.00	0.00
12.00	6.00	-6.00	12.00	0.00
14.00	7.05	-7.05	14.10	0.10
16.00	8.05	-8.05	16.10	0.10
18.00	9.05	-9.05	18.10	0.10
20.00	10.05	-10.05	20.10	0.10
22.00	11.05	-11.05	22.10	0.10
24.00	12.05	-12.05	24.10	0.10
26.00	13.05	-13.05	26.10	0.10
28.00	14.05	-14.05	28.10	0.10
30.00	15.05	-15.05	30.10	0.10
32.00	16.05	-16.10	32.15	0.15
34.00	17.05	-17.10	34.15	0.15
35.80	18.00	-18.00	36.00	0.20

The uncertainty of measurement was  $\pm 0.11$  inH<sub>2</sub>O

\*  $\Delta P$  = High-port side - Low-port side

\* UUC = Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor  $k = 2$ , providing a level of confidence of approximately 95 %.

-o0o-

เอกสารไม่ควบคุม





## Certificate of Calibration

Certificate No. : 24P1369

Page : 1 of 2

**Equipment :** Aneroid Barometer  
**Manufacturer:** Barigo  
**Model :** -  
**Serial No.:** -  
**ID No.:** UAE.ANV.013/2547

**Condition As-Received:** Used Item

**Received Date:** 05 April 2024

**Calibration Date:** 22 April 2024

**Reference:** 2404-0243WSC

**Ambient Temperature:** ( 23 ± 2 ) °C

**Relative Humidity:** ( 50 ± 15 ) %

**Atmospheric Pressure:** 1007 mbar

**Submitted by:** United Analyst and Engineering Consultant Co.,Ltd.

81 Soi Udomsuk 41, Sukhumvit Road, Bangchak,  
Phrakhanong, Bangkok 10260

**Procedure used:** The calibration was conducted by direct comparison method against Pressure Measuring Instruments Standard according to calibration procedure CP-P10, using " DKD-R 6-1 ; Calibration of Pressure Gauges " as a guidelines.

### Condition of this result of calibration

1.Reference standards instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Certificate No.</u>	<u>Due Date</u>
1) Standard Barometer	DPI142	1422505046	MP-0094-23	03 May 2024

2.This instrument was installed in vertical orientation and center of the dial was used as the reference level.

3.This result of calibration was made on requested at the point specified by customer.

4.Scale and conversion factor is 1 kPa = 7.50062 mmHg

5.This result of calibration instrument was in absolute pressure.

6.This instrument was used clean air as pressure media.

7.The certificate is valid only to the item calibrated on date and place of calibration.

8.This Certification is traceable to the International System of Unit maintained through:-

-National Institute of Metrology Thailand (NIMT)

**Calibrated by :** Suksan Khankaew  
**Issue Date :** 23 April 2024

**Approved Signatory :** \_\_\_\_\_  
[ ] Phalinee Prabpaipal  
[ ] Sura Suwannasri  
[✓] Attapol Panurach

เอกสารไม่ควบคุม



Cert.No.: 24P1369

Page: 2 of 2

**Result of calibration:- Without adjustment**

**Range :** 720 mmHg to 780 mmHg

**Function:- Absolute Pressure Measurement**

**Scale Interval :** 1 mmHg ( The Fifth Estimate )

**Increasing Pressure**

Applied Pressure (mmHg)	718.40	729.71	740.61	751.07	761.97	773.05	786.91
UUC* Indication (mmHg)	720.0	730.0	740.0	750.0	760.0	770.0	780.0
Error (mmHg)	1.60	0.29	-0.61	-1.07	-1.97	-3.05	-6.91

**Decreasing Pressure**

Applied Pressure (mmHg)	786.91	772.99	761.71	750.69	740.13	729.35	718.44
UUC* Indication (mmHg)	780.0	770.0	760.0	750.0	740.0	730.0	720.0
Error (mmHg)	-6.91	-2.99	-1.71	-0.69	-0.13	0.65	1.56

The uncertainty of measurement was  $\pm 0.24$  mmHg

\* UUC = Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor  $k = 2$ , providing a level of confidence of approximately 95 %.

-oOo-

เอกสารไม่ควบคุม





## Certificate of Calibration

Certificate No. : 24H753

Page : 1 of 2

Equipment : Dial Thermo-Hygrometer

Manufacturer: Barigo

Model : -

Serial No.: -

ID No.: UAE.ANV.127/2550

Condition As-Received: Used Item

Received Date: 05 April 2024

Calibration Date: 10 April 2024  
to 18 April 2024

Reference: 2404-0247WSC

Ambient Temperature: ( 25 ± 3 ) °C

Relative Humidity: ( 50 ± 20 ) %

This certificate may not be reproduced other than in full,  
except with the prior written approval of the head of  
Corporate Services 3: Equipment Calibration and Testing Services.

Submitted by: United Analyst and Engineering Consultant Co.,Ltd.

81 Soi Udomsuk 41, Sukhumvit Road,  
Bangchak, Phrakhanong, Bangkok 10260

Procedure used: Calibration were conducted using in-house calibration procedure CP-H02 according to comparison with standard chilled mirror sensor for humidity measurement function and comparison with standard temperature probe for temperature measurement function into humidity / temperature chamber.

### Condition of this result of calibration

1.Reference standards instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Certificate No.</u>	<u>Due Date</u>
1) Chilled Mirror Hygrometer	Dew Master	44730	21656	02 Aug 2024
2) Handheld Thermometer With Sensor	1521	A5A339	2311238	16 Oct 2024

2.The certificate is valid only to the item calibrated on date and place of calibration.

3.This Certification is traceable to the International System of Unit maintained through:-

- Thunder Scientific Corporation, NVLAB Accreditation No. Calibration 200582-0
- Technology Promotion Association (Thailand-Japan), NSC-ONSC Accredited No. Calibration 0008

Calibrated by : Chakrit Waewwanjua  
Issue Date : 18 April 2024

Approved Signatory : \_\_\_\_\_  
[ ] Chakrit Waewwanjua  
[✓] Viporn Tantiyawutti  
[ ] Unnopphol Harachai

เอกสารไม่ควบคุม

### MULTI-POINT GAS TEST REPORT

**Test Date** : Sep 17, 2024

**Equipment** : Gas Analyzer (NO<sub>2</sub>)

**Model** : 42i

**Manufacturer** : Thermo Scientific

**Serial Number** : CM08130002

#### Standard Gas Concentration

Sulphur Dioxide (SO <sub>2</sub> )	42.89
Nitric Oxide (NO)	46.77
Methane (CH <sub>4</sub> )	-
Carbon Monoxide (CO)	965.9
Cylinder No. :	EB0159156
Expiration Date :	Nov 6, 2026


#### Dilutor Detail

Manufacturer :	Thermo Scientific
Model :	146i
Serial Number :	1180540071

#### Multi-point gas test data

	Reference Value (ppb)		Analyzer Display (ppb)	Difference Error	Percent Error	[% Error]
Level 1	Zero	0.0	0.5	0.50	0.50	0.50
Level 2	20.00%	100.0	101.6	1.60	1.57	1.57
Level 3	40.00%	200.0	200.5	0.50	0.25	0.25
Level 4	60.00%	300.0	300.8	0.80	0.27	0.27
Level 5	80.00%	400.0	400.0	0.00	0.00	0.00
Remark : Measuring Range 500.0 ppb				Average Difference (%)		0.52

:Acceptable Limit  $\pm 5\%$

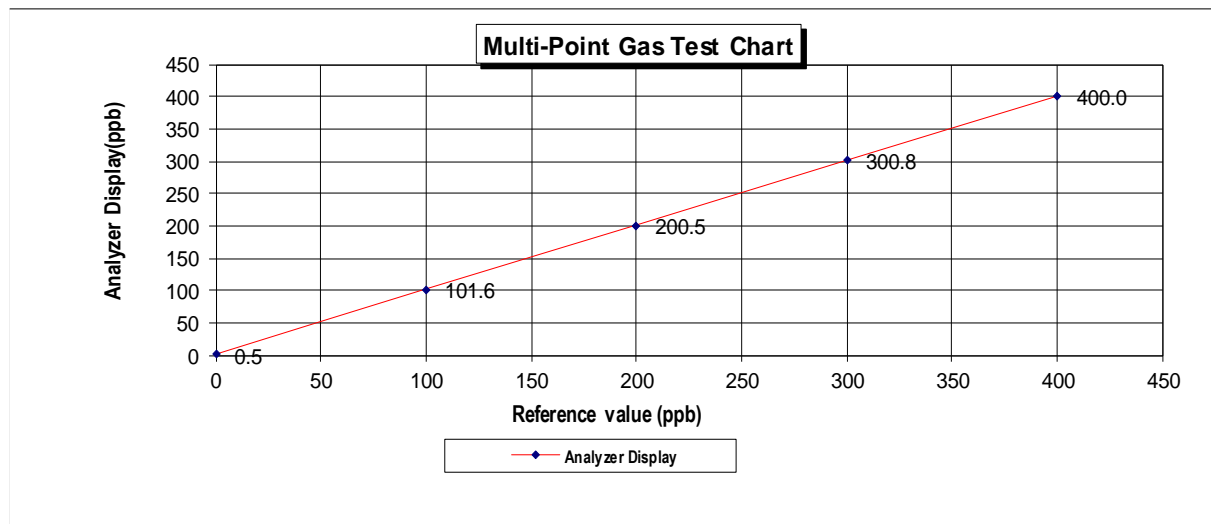

**Calculate by**

*Sirichai G.*  
.....  
17 / 9 / 2567

**Approve by**

*P. K. K.*  
.....  
17 / Sep / 2024



Cert. No.: 24H753

Page.: 2 of 2

**Result of Calibration:-** Without Adjustment

**Function:** Humidity Measurement.

<u>Reference Temperature</u> (°C)	<u>Standard Humidity</u> (%R.H.)	<u>UUC* Reading</u> (%R.H.)	<u>Error</u> (%R.H.)	<u>Uncertainty of Measurement</u> (±%R.H.)
25.0	40.1	43	2.9	1.6
25.0	60.0	60	0.0	1.7
25.0	80.0	78	-2.0	1.8

**Result of Calibration:-** Without Adjustment

**Function:** Temperature Measurement.

<u>Standard Temperature</u> (°C)	<u>UUC* Reading</u> (°C)	<u>Error</u> (°C)	<u>Uncertainty of Measurement</u> (±°C)
20.014	20.0	-0.014	0.72
25.033	25.0	-0.033	0.72
30.010	30.0	-0.010	0.72
35.027	34.5	-0.527	0.72
40.013	39.5	-0.513	0.72

**UUC\* :** Unit Under Calibration

The reported uncertainty of measurement was base on standard uncertainty multiplied by coverage factor  $k = 2.00$ , providing confidence level approximately 95%.

-o0o-

เอกสารไม่ควบคุม



### MULTI-POINT GAS TEST REPORT

**Test Date** : Sep 20,2024

**Equipment** : Gas Analyzer (NO<sub>2</sub>)

**Model** : 42i

**Manufacturer** : Thermo Scientific

**Serial Number** : CM19050148

#### Standard Gas Concentration

Sulphur Dioxide (SO <sub>2</sub> )	42.89
Nitric Oxide (NO)	46.77
Methane (CH <sub>4</sub> )	-
Carbon Monoxide (CO)	965.9
Cylinder No. :	EB0159156
Expiration Date :	Nov 6,2026


#### Dilutor Detail

Manufacturer :	Thermo Scientific
Model :	146i
Serial Number :	1180540071

#### Multi-point gas test data

Reference Value (ppb)			Analyzer Display (ppb)	Difference Error	Percent Error	[% Error ]
Level 1	Zero	0.0	0.0	0.00	0.00	0.00
Level 2	20.00%	100.0	100.7	0.70	0.70	0.70
Level 3	40.00%	200.0	200.6	0.60	0.30	0.30
Level 4	60.00%	300.0	300.9	0.90	0.30	0.30
Level 5	80.00%	400.0	400.0	0.00	0.00	0.00
Remark : Measuring Range 500.0 ppb				Average Difference (%)		0.26

Multi-Point Gas Test Chart

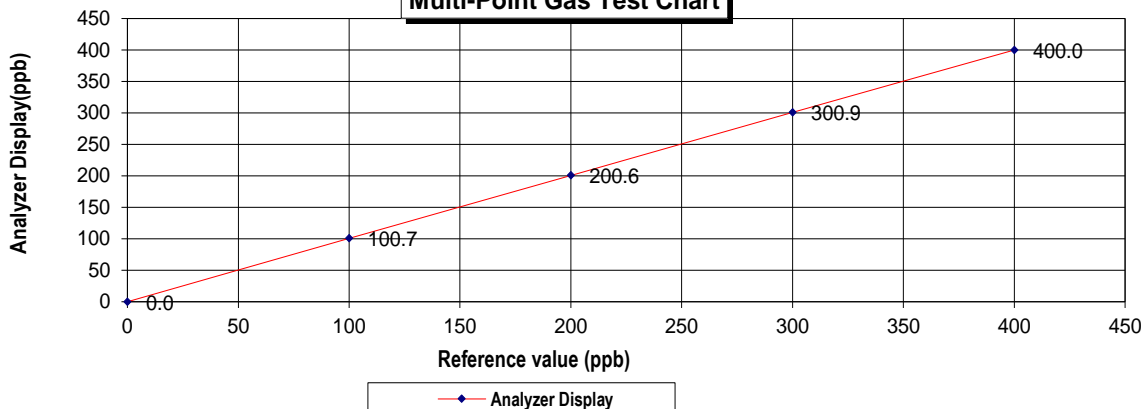

Calculate by

20 / 9 / 2567

Approve by

20 / Sep / 2024

### MULTI-POINT GAS TEST REPORT

**Test Date** : Sep 17, 2024

**Equipment** : Gas Analyzer (NO<sub>2</sub>)

**Model** : 42i

**Manufacturer** : Thermo Scientific

**Serial Number** : CM19050149

#### Standard Gas Concentration

Sulphur Dioxide (SO <sub>2</sub> )	42.89
Nitric Oxide (NO)	46.77
Methane (CH <sub>4</sub> )	-
Carbon Monoxide (CO)	965.9
Cylinder No. :	EB0159156
Expiration Date :	Nov 06, 2026


#### Dilutor Detail

Manufacturer :	Thermo Scientific
Model :	146i
Serial Number :	1180540071

#### Multi-point gas test data

Reference Value (ppb)			Analyzer Display (ppb)	Difference Error	Percent Error	[% Error ]
Level 1	Zero	0.0	0.0	0.00	0.00	0.00
Level 2	20.00%	100.0	100.8	0.80	0.79	0.79
Level 3	40.00%	200.0	200.6	0.60	0.30	0.30
Level 4	60.00%	300.0	300.7	0.70	0.23	0.23
Level 5	80.00%	400.0	400.0	0.00	0.00	0.00
Remark : Measuring Range 500.0 ppb				Average Difference (%)		0.27

Multi-Point Gas Test Chart

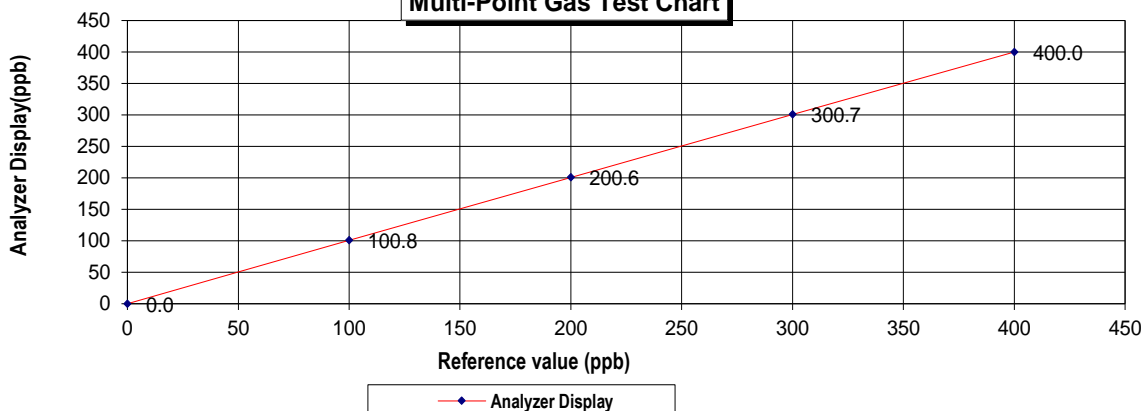

Calculate by

17 / 9 / 2567

Approve by

17 / Sep / 2024

## CERTIFICATE OF ANALYSIS

### Grade of Product: EPA PROTOCOL STANDARD

Customer: AIR LIQUIDE (THAILAND)

LTD

Part Number: E05NI91E15A0014

Cylinder Number: EB0162121

Laboratory: 124 - Plumsteadville - PA

PGVP Number: A12023

Gas Code: CO,CO<sub>2</sub>,NO,NO<sub>2</sub>,SO<sub>2</sub>,BALN

Reference Number: 160-402772205-1

Cylinder Volume: 144.0 CF

Cylinder Pressure: 2016 PSIG

Valve Outlet: 660

Certification Date: Jul 06, 2023

Expiration Date: Jul 06, 2031

Certification performed in accordance with "EPA Traceability Protocol for Assay and Certification of Gaseous Calibration Standards" (May 2012) document EPA 800/R-12/531, using the assay procedures listed. Analytical Methodology does not require correction for analytical interference. This cylinder has a total analytical uncertainty as stated below with a confidence level of 95%. There are no significant impurities which affect the use of this calibration mixture. All concentrations are on a mole/mole basis unless otherwise noted. The results relate only to the items tested. The report shall not be reproduced except in full without approval of the laboratory. Do Not Use This Cylinder below 100 psig, i.e. 0.7 megapascals.

#### ANALYTICAL RESULTS

Component	Requested Concentration	Actual Concentration	Protocol Method	Total Relative Uncertainty	Assay Dates
NOX	100.0 PPM	100.4 PPM	G1	+/- 0.9% NIST Traceable	06/27/2023, 07/06/2023
NITRIC OXIDE	100.0 PPM	100.2 PPM	G1	+/- 0.9% NIST Traceable	06/27/2023, 07/06/2023
SULFUR DIOXIDE	100.0 PPM	100.0 PPM	G1	+/- 1.4% NIST Traceable	06/27/2023, 07/06/2023
CARBON MONOXIDE	200.0 PPM	199.2 PPM	G1	+/- 0.3% NIST Traceable	06/26/2023
CARBON DIOXIDE	8.000 %	7.982 %	G1	+/- 1.2% NIST Traceable	06/27/2023
NITROGEN	Balance				

#### CALIBRATION STANDARDS

Type	Lot ID	Cylinder No	Concentration	Uncertainty	Expiration Date
GMIS	104202308	CC754364	98.36 PPM NITRIC OXIDE/NITROGEN	+/- 0.4%	Jan 04, 2031
PRM	C2219101	APE1514048	100.19 PPM NITRIC OXIDE/NITROGEN	+/- 0.3%	Feb 28, 2025
GMIS	2023042525	CC754381	98.52 PPM NITRIC OXIDE/NITROGEN	+/- 0.4%	Apr 25, 2031
PRM	12409	D913660	15.01 PPM NITROGEN DIOXIDE/AIR	+/- 1.5%	Feb 17, 2023
GMIS	153400202002	EB0130037	9.693 PPM NITROGEN DIOXIDE/NITROGEN	+/- 1.6%	Sep 29, 2025
NTRM	160102-22	KAL003820	97.69 PPM SULFUR DIOXIDE/NITROGEN	+/- 0.8%	Nov 01, 2027
CO	230601	CC745902	249.47 PPM CARBON MONOXIDE/NITROGEN	+/- 0.3%	Dec 09, 2028
NTRM	130606-02	CC411730	13.359 % CARBON DIOXIDE/NITROGEN	+/- 0.6%	May 14, 2025

The SRM, NTRM, PRM, or RGM noted above is only in reference to the GMIS used in the assay and not part of the analysis.

#### ANALYTICAL EQUIPMENT

Instrument/Make/Model	Analytical Principle	Last Multipoint Calibration
Nicolet iS50 FTIR AUP2010245 CO <sub>2</sub>	FTIR	Jun 15, 2023
SIEMENS ULTRAMAT6E N1-C8-180	NDIR	Jun 14, 2023
Nicolet iS50 FTIR AUP2010245 NO	FTIR	Jun 29, 2023
Nicolet iS50 FTIR AUP2010245 NO <sub>2</sub>	FTIR	Jun 15, 2023
Nicolet iS50 FTIR AUP2010245 SO <sub>2</sub>	FTIR	Jun 08, 2023

  
Approved for Release

### MULTI-POINT GAS TEST REPORT

**Test Date** : Sep 6, 2024

**Equipment** : Gas Analyzer (SO<sub>2</sub>)

**Model** : 43i

**Manufacturer** : Thermo SCIENTIFIC

**Serial Number** : CM22387061

#### Standard Gas Concentration

Sulphur Dioxide (SO <sub>2</sub> )	42.89
Nitric Oxide (NO)	46.77
Methane (CH <sub>4</sub> )	-
Carbon Monoxide (CO)	965.9
Cylinder No. :	EB01159156
Expiration Date :	Nov 06, 2026


#### Dilutor Detail

Manufacturer :	Thermo SCIENTIFIC
Model :	146i
Serial Number :	1180540071

#### Multi-point gas test data

	Reference Value (ppb)		Analyzer Display (ppb)	Difference Error	Percent Error	[% Error]
Level 1	Zero	0.0	0.0	0.00	0.00	0.00
Level 2	20.00%	100.0	100.7	0.70	0.70	0.70
Level 3	40.00%	200.0	200.7	0.70	0.35	0.35
Level 4	60.00%	300.0	301.1	1.10	0.37	0.37
Level 5	80.00%	400.0	400.0	0.00	0.00	0.00
Remark : Measuring Range			500.0 ppb	Average Difference (%)		0.28
:Acceptable Limit $\pm$ 5%						

Multi-Point Gas Test Chart

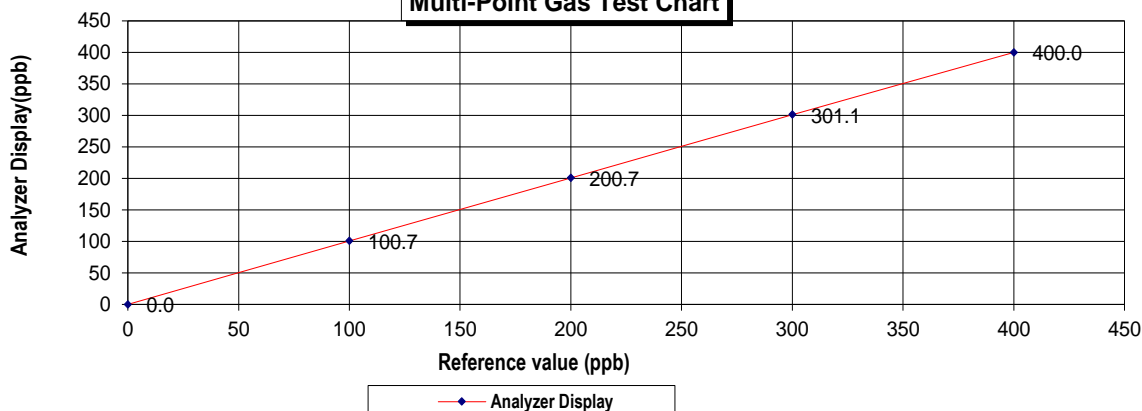

Calculate by

6 / 9 / 2567

Approve by

6 / Sep / 2024

### MULTI-POINT GAS TEST REPORT

**Test Date : June 19, 2024**

**Equipment :** Gas Analyzer (SO<sub>2</sub>)

**Model :** 43i

**Manufacturer :** Thermo SCIENTIFIC

**Serial Number :** CM22387063

#### Standard Gas Concentration

Sulphur Dioxide (SO <sub>2</sub> )	42.89
Nitric Oxide (NO)	46.77
Methane (CH <sub>4</sub> )	-
Carbon Monoxide (CO)	965.9
Cylinder No. :	EB0159156
Expiration Date :	Nov 06, 2026


#### Dilutor Detail

Manufacturer :	Thermo SCIENTIFIC
Model :	146i
Serial Number :	1180540071

#### Multi-point gas test data

	Reference Value (ppb)		Analyzer Display (ppb)	Difference Error	Percent Error	[% Error ]
Level 1	Zero	0.0	0.0	0.00	0.00	0.00
Level 2	20.00%	100.0	100.8	0.80	0.79	0.79
Level 3	40.00%	200.0	200.7	0.70	0.35	0.35
Level 4	60.00%	300.0	301.1	1.10	0.37	0.37
Level 5	80.00%	400.0	400.0	0.00	0.00	0.00
Remark : Measuring Range 500.0 ppb				Average Difference (%)		0.30

:Acceptable Limit  $\pm 5\%$

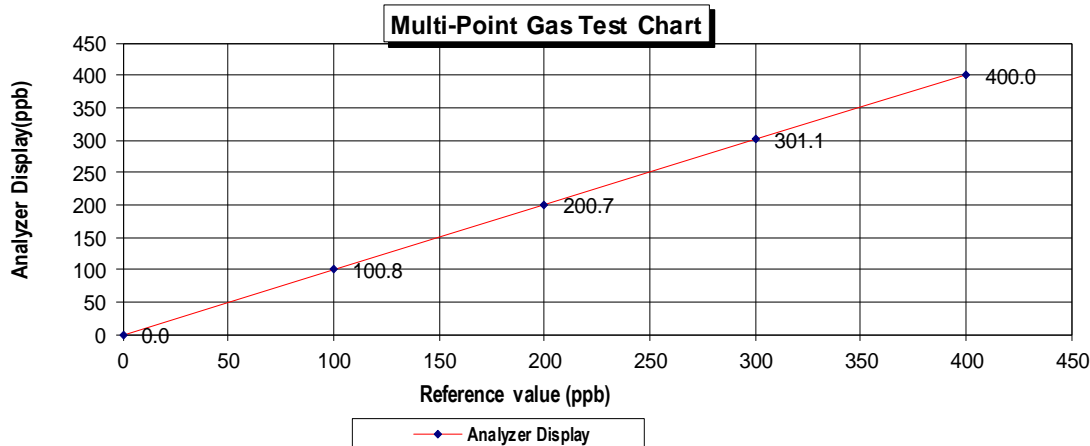

**Calculate by**

*Sirchai S.*

19 / 06 / 2567

**Approve by**

*Pattana K.*

19 / June / 2024



### MULTI-POINT GAS TEST REPORT

**Test Date** : May 15, 2024

**Equipment** : Gas Analyzer (SO<sub>2</sub>)

**Model** : 43i

**Manufacturer** : Thermo SCIENTIFIC

**Serial Number** : CM22387067

#### Standard Gas Concentration


Sulphur Dioxide (SO <sub>2</sub> )	44.68
Nitric Oxide (NO)	45.94
Methane (CH <sub>4</sub> )	-
Carbon Monoxide (CO)	984.8
Cylinder No. :	EB0143262
Expiration Date :	Jun 24, 2024

#### Dilutor Detail

Manufacturer :	Thermo SCIENTIFIC
Model :	146i
Serial Number :	1180540071

#### Multi-point gas test data

Reference Value (ppb)			Analyzer Display (ppb)	Difference Error	Percent Error	[% Error ]
Level 1	Zero	0.0	0.9	0.90	0.90	0.90
Level 2	20.00%	100.0	100.8	0.80	0.79	0.79
Level 3	40.00%	200.0	200.9	0.90	0.45	0.45
Level 4	60.00%	300.0	300.9	0.90	0.30	0.30
Level 5	80.00%	400.0	400.0	0.00	0.00	0.00
Remark : Measuring Range 500.0 ppb				Average Difference (%)		0.49

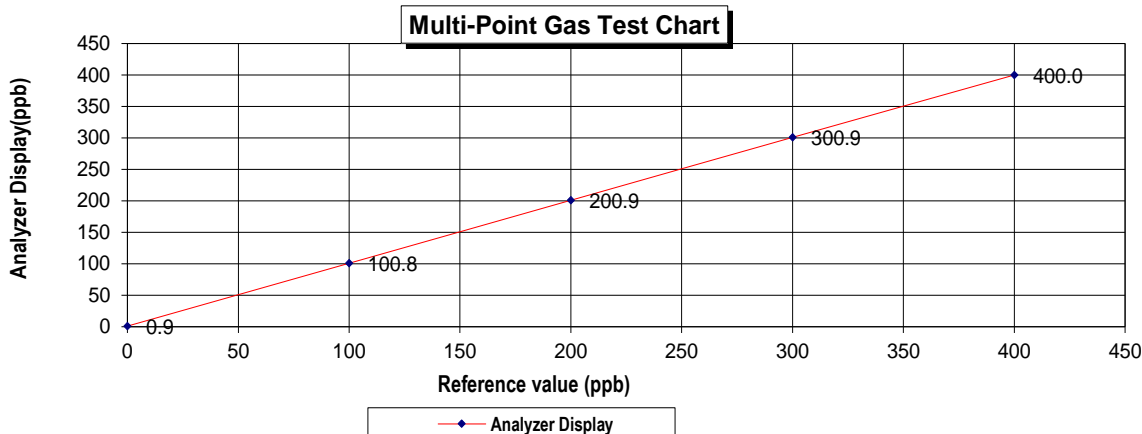

Calculate by

*Sirichai G.*  
.....15...../.....05...../.....2567.....

Approve by

*P. K.*  
.....15...../.....May...../.....2024.....

## CERTIFICATE OF ANALYSIS

### Grade of Product: EPA PROTOCOL STANDARD

Customer: AIR LIQUIDE (THAILAND)

LTD

Part Number: E05NI91E15A0014

Cylinder Number: EB0162121

Laboratory: 124 - Plumsteadville - PA

PGVP Number: A12023

Gas Code: CO,CO<sub>2</sub>,NO,NO<sub>x</sub>,SO<sub>2</sub>,BALN

Reference Number: 160-402772205-1

Cylinder Volume: 144.0 CF

Cylinder Pressure: 2016 PSIG

Valve Outlet: 660

Certification Date: Jul 06, 2023

Expiration Date: Jul 06, 2031

Certification performed in accordance with "EPA Traceability Protocol for Assay and Certification of Gaseous Calibration Standards" (May 2012) document EPA 800/R-12/531, using the assay procedures listed. Analytical Methodology does not require correction for analytical interference. This cylinder has a total analytical uncertainty as stated below with a confidence level of 95%. There are no significant impurities which affect the use of this calibration mixture. All concentrations are on a mole/mole basis unless otherwise noted. The results relate only to the items tested. The report shall not be reproduced except in full without approval of the laboratory. Do Not Use This Cylinder below 100 psig, i.e. 0.7 megapascals.

#### ANALYTICAL RESULTS

Component	Requested Concentration	Actual Concentration	Protocol Method	Total Relative Uncertainty	Assay Dates
NOX	100.0 PPM	100.4 PPM	G1	+/- 0.9% NIST Traceable	06/27/2023, 07/06/2023
NITRIC OXIDE	100.0 PPM	100.2 PPM	G1	+/- 0.9% NIST Traceable	06/27/2023, 07/06/2023
SULFUR DIOXIDE	100.0 PPM	100.0 PPM	G1	+/- 1.4% NIST Traceable	06/27/2023, 07/06/2023
CARBON MONOXIDE	200.0 PPM	199.2 PPM	G1	+/- 0.3% NIST Traceable	06/26/2023
CARBON DIOXIDE	8.000 %	7.982 %	G1	+/- 1.2% NIST Traceable	06/27/2023
NITROGEN	Balance				

#### CALIBRATION STANDARDS

Type	Lot ID	Cylinder No	Concentration	Uncertainty	Expiration Date
GMIS	104202308	CC754364	98.36 PPM NITRIC OXIDE/NITROGEN	+/- 0.4%	Jan 04, 2031
PRM	C2219101	APE1514048	100.19 PPM NITRIC OXIDE/NITROGEN	+/- 0.3%	Feb 28, 2025
GMIS	2023042525	CC754381	98.52 PPM NITRIC OXIDE/NITROGEN	+/- 0.4%	Apr 25, 2031
PRM	12409	D913660	15.01 PPM NITROGEN DIOXIDE/AIR	+/- 1.5%	Feb 17, 2023
GMIS	153400202002	EB0130037	9.693 PPM NITROGEN DIOXIDE/NITROGEN	+/- 1.6%	Sep 29, 2025
NTRM	160102-22	KAL003820	97.69 PPM SULFUR DIOXIDE/NITROGEN	+/- 0.8%	Nov 01, 2027
CO	230601	CC745902	249.47 PPM CARBON MONOXIDE/NITROGEN	+/- 0.3%	Dec 09, 2028
NTRM	130606-02	CC411730	13.359 % CARBON DIOXIDE/NITROGEN	+/- 0.6%	May 14, 2025

The SRM, NTRM, PRM, or RGM noted above is only in reference to the GMIS used in the assay and not part of the analysis.

#### ANALYTICAL EQUIPMENT

Instrument/Make/Model	Analytical Principle	Last Multipoint Calibration
Nicolet iS50 FTIR AUP2010245 CO <sub>2</sub>	FTIR	Jun 15, 2023
SIEMENS ULTRAMAT6E N1-C8-180	NDIR	Jun 14, 2023
Nicolet iS50 FTIR AUP2010245 NO	FTIR	Jun 29, 2023
Nicolet iS50 FTIR AUP2010245 NO <sub>2</sub>	FTIR	Jun 15, 2023
Nicolet iS50 FTIR AUP2010245 SO <sub>2</sub>	FTIR	Jun 08, 2023

  
Approved for Release

## Certificate of Calibration

### Customer

Name : UNITED ANALYST AND ENGINEERING  
CONSULTANT CO.,LTD.  
Address : 81 Soi Udomsuk 41, Sukhumvit Road, Bangchak,  
Prakanong, Bangkok 10260

Certificate No : 24-ACT-091  
Request No : Req-2024-1380

### Unit Under Calibration Details

Measurement item : Acoustic Calibrator Class : 1  
Manufacturer : SVANTEK Range : 94 , 114 dB / 1000 Hz  
Model : SV 36 Instrument Status : Used  
Serial Number : 107224  
ID : UAE.EFM.171/2564

### Calibration Environment and Details


Temperature : ( 23 ±2 °C )  
Humidity : ( 50 ± 20 %RH )  
Barometric Pressure : ( 1013 ±10.0 hPa )  
Received Date : 24 June 2024  
Calibration Date : 26 June 2024  
Location of Calibration : LAB 1 Acoustic  
Calibration Procedure : In-house method CP-ACT-02 based on IEC 60942:2017 Electroacoustics - Sound calibrators


Reference Standard	Model	Serial Number	Traceable	Due Calibration
Sound Calibrator	SV 35A	58079	EEI	12 June 2025
THD Multimeter	2015	1047765	NIMT	16 January 2025

**Traceability** : This certificate provides traceability of measurement to recognized national standard, and to the realization of the international System of Units (SI).

### Note

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor  $k=2$ , providing a level of confidence approximately 95 %.

Calibrated By :   
Mr. Noppadon Luangart  
Service Calibration Engineer

Approved By :   
Mr. Pacit Mathavorn  
Calibration Engineer Supervisor

Issue Date : 26 June 2024



Certificate No : 24-ACT-091

Request No : Req-2024-1380

Sound pressure level

Calibration Results : Without Adjustment

Calibration Range (dB)	Without Adjustment (dB)		Adjustment (dB)		Uncertainty ( ± dB)	Acceptance limit Class 1 ( ± dB)	Result
	Measured	Deviated value	Measured	Deviated value			
94 dB / 1000 Hz	94.02	0.02	-	-	0.14	0.25	Pass
114 dB / 1000 Hz	114.05	0.05	-	-	0.13	0.25	Pass

Frequency of Sound pressure level

Calibration Range (Hz)	Without Adjustment		Adjustment		Uncertainty ( ± %)	Acceptance limit Class 1 ( ± %)	Result
	Measured (Hz)	Deviated	Measured (Hz)	Deviated			
94 dB / 1000 Hz	1000.00	0.00	-	-	0.01	0.70	Pass
114 dB / 1000 Hz	1000.00	0.00	-	-	0.01	0.70	Pass

Total Harmonic Distortion plus Noise of Sound pressure level (THD+N %)

Calibration Range (Hz)	Without Adjustment	Adjustment	Uncertainty ( ± %)	Acceptance limit Class 1 ( ± %)	Result
	Measured (%)	Measured (%)			
94 dB / 1000 Hz	0.24	-	0.40	2.5	Pass
114 dB / 1000 Hz	0.44	-	0.40	2.5	Pass

Note :

Function	Maximum-permitted Uncertainty of measurement
Sound pressure level	0.15 dB
Frequency	0.20%
Total distortion+noise	0.50%

- Acceptance limit was IEC60942:2017 Class 1

- The calibration results exclude the calibrator pressure correction

- The calibration results exclude the microphone volume correction

Certificate No : 24-ACT-091

Request No : Req-2024-1380

### Decision Rule for Statements of Conformity


The standard decision rule employed for the statements of conformity to each calibration result will be applied using ILAC-G8:09:2019, Guidelines on the Reporting of Compliance with Specification as following Fig. and statements

Pass = The measurement result plus the expanded uncertainty with a 95% coverage probability were within the limit.

Pass<sup>1</sup> = The measurement result was within the limit. However, a portion of the expanded uncertainty of measurement at 95% exceeds the limit.

Fail<sup>1</sup> = The measurement result was out of the limit. However, a portion of the expanded uncertainty of measurement at 95% is within the limit.

Fail = The measurement result plus the expanded uncertainty with a 95% coverage probability were outside the limit.

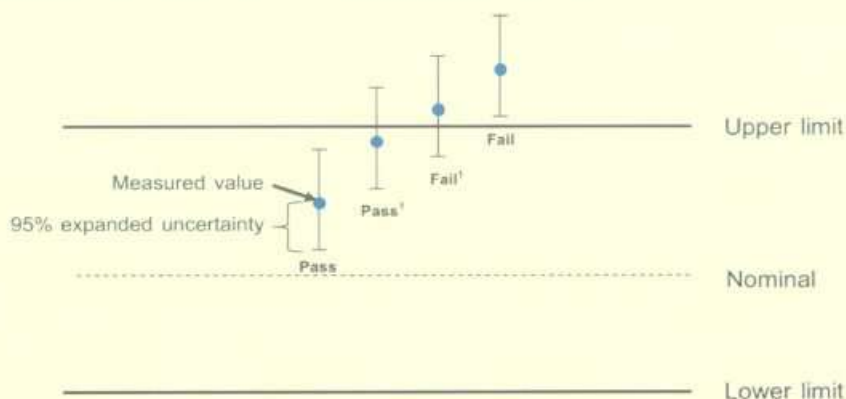

End of Calibration





**ELECTRICAL AND ELECTRONICS INSTITUTE  
FOUNDATION FOR INDUSTRIAL DEVELOPMENT**

975 Moo 4, Bangpoo Industrial Estate, Soi 8, Sukhumvit Road km 37,

Phraek Sa, Mueang Samut Prakan, Samut Prakan 10280

Tel: +66 2709 4860 Fax: +66 2324 0917



Certificate No.: CP20240292EA

Operation No.: CP2024070255

## Certificate of Calibration

**Equipment:** Sound Level Meter

**Manufacturer:** Larson Davis (Meter), PCB (Microphone), PCB (Preamplifier)

**Model/Type:** LxT2 (Meter), 375B02 (Microphone), PRMLxT2B (Preamplifier)

**Serial No.:** 0005348 (Meter), 11800 (Microphone), 056140 (Preamplifier)

**ID No.:** UAE.EFM.045/2563

**Customer:** United Analyst and Engineering Consultant Co.,Ltd.

**Address:** 81 Soi Udomsuk 41, Sukhumvit Road, Bangchak  
Phrakhanong, Bangkok 10260

**Received Date:** 25 July 2024

**Calibrated Date:** 6 - 7 August 2024

**Issued Date:** 7 August 2024

**Calibrated by:** Ms. Juntaporn Kunhakom

**Approved by:**

( Mr. Sittichai Swaksuriyawong )

Group Manager

This report was prepared electronically using applicable electronic signature. Printing or copy of file are considered as a copy of the document.

The reported uncertainty of measurement was based on standard uncertainty multiplied by a coverage factor ( $k$ ) providing a level of confidence of approximately 95%. This certificate may not be reproduced other than in full except with the prior written approval of the Electrical and Electronics Institute, Foundation for Industrial Development.

Certificate No.: CP20240292EA

### Calibration Report

**Equipment:** Sound Level Meter  
**Manufacturer:** Larson Davis (Meter), PCB (Microphone), PCB (Preamplifier)  
**Model/Type:** LxT2 (Meter), 375B02 (Microphone), PRMLxT2B (Preamplifier)  
**Serial No.:** 0005348 (Meter), 11800 (Microphone), 056140 (Preamplifier)  
**ID No.:** UAE.EFM.045/2563  
**Ambient Temperature:** ( 23 ± 2 ) °C  
**Relative Humidity:** ( 50 ± 15 ) %  
**Pressure:** (101.3 ± 1.5) kPa  
**Method of Calibration :-**  
IEC 61672-3:2013.

#### Condition of this result of calibration

1. Reference standards instrument :-

Instrument	Model	Serial No.	Cert. No.	Due Date
1) Standard microphone	4180	2787490	AA-1012-23	12 November 2024
2) Arbitrary Function Generator	AFG2021	C010063	CK20240048EA	23 June 2025
3) Programmable Attenuator	PA5	2755	EF-0040-23	1 October 2024
4) 6.5 Digit precision multimeter	8846A	9610014	CB20230200EA	15 November 2024
5) Pressure humidity and Temperature Transmitter	PTU301	L3950483	CL1-P240023 CD20240142EA	24 March 2025 12 June 2025
6) Pressure humidity and Temperature Transmitter	PTU301	L3950484	CL1-P240030 CD20240143EA	11 April 2025 12 June 2025
7) Performance Audio Analyzer	U8903B	MY56510003	CB20240035EB CK20230072EA	13 February 2025 13 September 2024

2. This result of calibration was found accurate as shown on date and place of calibration only.

3. This certification is traceable to the international system of unit maintained at :-

Reference standards instrument for Acoustic function

- National Institute of Metrology (Thailand)

Reference standards instrument for Electrical function

- National Institute of Metrology (Thailand)

- Electrical and Electronics Institute; NSC Accredited Calibration No.0119

#### Result of Calibration:-

Function : 1. Indication at the calibration check frequency

Reference Acoustic Signal (dB)	Measured value (dB)	Deviation (dB)	Acceptance limits (dB)
-	-	-	-

Certificate No.: CP20240292EA

## Calibration Report

Function : 2. Self-generated Noise

### 2.1 Microphone Installed

Measured value (dB)
31.6

### 2.2 Microphone replaced by the electrical input signal device

Frequency Weighting	Measured value (dB)
A-weighting	31.5
C-weighting	31.6
Z-weighting	36.6

Function : 3. Acoustical signal tests of frequency weightings (Without Windscreen)

Meter free-field acoustic response at a level of 84 dB.

Frequency (Hz)	Deviation from various Frequency Weighting Response Curve			
	C-Weighting (dB)	A-Weighting (dB)	Z-Weighting (dB)	Acceptance limits (dB)
125	0.3	0.2	0.2	±1.5
1000	-0.2	-0.2	-0.2	±1.0
8000	2.9	2.9	2.9	±5.0

Function : 4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various Frequency Weighting Response Curve			
	C-Weighting (dB)	A-Weighting (dB)	Z-Weighting (dB)	Acceptance limits (dB)
63	0.0	0.0	0.0	±2.0
125	0.0	0.0	0.0	±1.5
250	0.0	0.0	0.0	±1.5
500	0.1	0.0	0.0	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.1	0.0	0.0	±2.0
4000	0.0	0.0	0.0	±3.0
8000	0.0	0.0	0.1	±5.0

Function : 5. Frequency and time weighting at 1 kHz

### 5.1 Frequency weighting at 1 kHz

Frequency Weighting	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
C-weighting	94.0	0.0	±0.2
A-weighting	94.0	0.0	±0.2
Z-weighting	94.0	0.0	±0.2

Certificate No.: CP20240292EA

### Calibration Report

#### 5.2 Time weighting at 1 kHz

Time Weighting	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
Fast	94.0	0.0	±0.1
Slow	94.0	0.0	±0.1
LAeq	94.0	0.0	±0.1

#### Function : 6. Long-Term Stability

Long-term stability over 30 minutes, with steady 1 kHz signal at reference level.

Time Period to Apply Signal (min)	Reference SPL (dB)	Record SPL at Conclusion of Time Period (dB)	Deviated value (dB)	Acceptance limits (dB)
30	94.0	94.0	0.0	±0.3

#### Function : 7. Level Linearity on the reference level range

##### 7.1 Level Linearity on the reference level range, Upper

Anticipated Value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
94.0	94.0	0.0	±1.1
99.0	99.0	0.0	±1.1
104.0	104.0	0.0	±1.1
109.0	109.0	0.0	±1.1
114.0	114.0	0.0	±1.1
119.0	119.0	0.0	±1.1
124.0	124.0	0.0	±1.1
129.0	129.0	0.0	±1.1
134.0	134.1	0.1	±1.1
139.0	139.1	0.1	±1.1
140.0	140.1	0.1	±1.1
141.0	141.1	0.1	±1.1
142.0	142.1	0.1	±1.1

Certificate No.: CP20240292EA

### Calibration Report

#### 7.2 Level Linearity on the reference level range, Lower

Anticipated Value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
94.0	94.0	0.0	±1.1
89.0	89.0	0.0	±1.1
84.0	84.0	0.0	±1.1
79.0	79.0	0.0	±1.1
74.0	74.0	0.0	±1.1
69.0	69.0	0.0	±1.1
64.0	64.0	0.0	±1.1
59.0	59.0	0.0	±1.1
54.0	54.0	0.0	±1.1
49.0	49.0	0.0	±1.1
44.0	44.1	0.1	±1.1
43.0	43.2	0.2	±1.1
42.0	42.3	0.3	±1.1
41.0	41.4	0.4	±1.1
40.0	40.5	0.5	±1.1

#### Function : 8. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
Fast	200	136.0	0.0	±1.0
	2	118.8	-0.2	+1.0 ; -2.5
	0.25	109.7	-0.3	+1.5 ; -5.0
Slow	200	129.5	-0.1	±1.0
	2	109.9	-0.1	+1.0 ; -5.0
LAE	200	130.0	0.0	±1.0
	2	110.0	0.0	+1.0 ; -2.5
	0.25	100.9	-0.1	+1.5 ; -5.0

#### Function : 9. Peak C sound level

Number of cycles in test signal	Anticipated Value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
Complete cycle	135.4	134.8	-0.6	±3.0
Positive half cycle	134.4	134.1	-0.3	±2.0
Negative half cycle	134.4	134.1	-0.3	±2.0

#### Function : 10. Overload indication

Measured value (dB)		Deviated value (dB)	Acceptance limits (dB)
Positive one-half cycle	Negative one-half cycle		
145.3	145.2	-0.1	±1.5

เอกสารไม่ควบคุม



Certificate No.: CP20240292EA

### Calibration Report

Function : 11. High-Level Stability

High-level stability over 5 minutes, with steady 1 kHz signal, 1 dB below upper boundary.

Time Period to Apply Signal (min)	Reference SPL (dB)	Record SPL at Conclusion of Time Period (dB)	Deviated value (dB)	Acceptance limits (dB)
5	139.0	139.0	0.0	±0.3

### Uncertainty of measurement

Function	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1) Indication at the calibration check frequency	0.30	Not applicable
2) Self-generated Noise	0.10	Not applicable
3) Acoustical signal tests of frequency weightings - Free-field sound pressure response level	0.30	0.60 (10Hz to 4kHz) 0.70 (>4kHz to 10kHz)
4) Electrical signal tests of frequency weightings	0.20	0.20
5) Frequency and time weighting at 1 kHz	0.20	0.20
6) Long-Term Stability	0.10	0.10
7) Level Linearity on the reference level range	0.30	0.30
8) Tone burst response	0.20	0.30
9) Peak C sound level	0.20	0.35
10) Overload indication	0.20	0.25
11) High-Level Stability	0.10	0.10

Remarks:

1. Indication at the calibration check frequency can not measured because customer does not provide a sound calibrator.
2. The acceptance limit is for the deviated value.
3. Acceptance limits was IEC61672-3:2013 Class 2.
4. The coverage factor  $k = 2.00$

- - End of Report - -



## Certificate of Calibration

### Customer

Name : UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.  
Address : 81 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Prakanong, Bangkok  
10260

Certificate No : 24-SLM-237

Request No : Req-2024-1456

### Unit Under Calibration Details

Measurement item : Sound Level Meter  
Microphone Class : 2  
Manufacturer : Larson Davis  
Microphone Model : 375A04  
Model : LxT2  
Microphone S/N : 329354  
Serial Number : 0005393  
Preamplifier Model : PRMLxT2C  
ID : UAE.EFM.030/2564  
Preamplifier S/N : 073808  
Resolution : 0.1 dB  
Instrument Status : Used

### Calibration Environment and Details


Temperature : 23 °C ± 2 °C  
Humidity : 50 %RH ± 20 %RH  
Barometric Pressure : 1013 hPa ± 10 hPa  
Received Date : 1 July 2024  
Calibrated Date : 10 July 2024  
Calibration Procedure : In-house method CP-SLM-01 based on IEC 61672-3 : 2013 Electroacoustics - Sound level meters - Part 3: Periodic tests  
Location of Calibration : Lab Acoustic


### Reference Standard

Instrument	Brand	Model	SN.	Due calibration	Traceability
Standard Microphone	GRAS	40AN	188273	20 August 2024	GRAS
Multifrequency Calibrator	Quest	Quest-cal	EFA000234	26 July 2024	TSI
Audio Generator	Svantek	Svan401	131	8 October 2024	WK Electric

### Note

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor  $k = 2$ , providing a level of confidence approximately 95 %.

Calibrated By :   
Mr. Noppadon Luangart  
Service Calibration Engineer

Approved By :   
Mr. Pacit Mathavorn  
Calibration Engineer Supervisor

Issue Date : 10 July 2024

Certificate No : 24-SLM-237

Request No : Req-2024-1456

1. Indication at the calibration check frequency

UUC Setting	Nominal	Before Adjust		After Adjust		UNCERTAINTY  ( ± dB)	Acceptance Limit ( ± dB)	Result
FAST / A / 37-139	Level (dB)	UUC	ERR	UUC	ERR			
Calibrator Setting		(dB)	(dB)	(dB)	(dB)			
1000 Hz 114 dB	113.76	114.3	0.54	113.8	+0.04	0.20	0.30	Pass

Note : Absolute sensitivity was established by the use of Sound Calibrator Brand SVANTEK, Model SV 35A, SN, 58079

2. Self-generated noise, Microphone installed

UUC Setting	Measured	UNCERTAINTY
FAST / 37-139		
UUC Weighting	(dB)	( ± dB)
A	28.7	0.10

3. Self-generated noise, Microphone replaced by the electrical input signal device

UUC Setting	Measured	UNCERTAINTY
FAST / 37-139		
UUC Weighting	(dB)	( ± dB)
A	28.4	0.10
C	28.4	0.10
Z	32.9	0.10

4. Acoustic signal test of frequency weightings (Without Windscreen)

UUC Setting	Deviation from various Frequency Weighting Response curve			UNCERTAINTY  ( ± dB)	Acceptance Limit ( ± dB)	Result
	A	C	Z			
FAST / 37-139	(dB)	(dB)	(dB)	0.60 0.60 0.60 0.70	1.5 1.0 3.0 5.0	Pass Pass Pass Pass
STD Setting	(dB)	(dB)	(dB)			
125 Hz	0.0	0.1	0.1			
1000 Hz	0.0	0.0	0.0			
4000 Hz	0.6	0.6	0.6			
8000 Hz	0.3	0.3	0.4			

Certificate No : 24-SLM-237

Request No : Req-2024-1456

5. Electrical signal test of frequency weightings, Weighting network response with relative to 1 kHz

UUC Setting	Deviation from various Frequency			UNCERTAINTY	Acceptance	Result
FAST / 37-139	Weighting Response curve				Limit	
STD Setting	A (dB)	C (dB)	Z (dB)	( ± dB)	( ± dB)	
63 Hz	-0.1	0.0	0.0	0.20	2.0	Pass
125 Hz	-0.1	0.0	0.0		1.5	Pass
250 Hz	-0.1	0.0	0.0		1.5	Pass
500 Hz	0.0	0.0	0.0		1.5	Pass
1000 Hz	0.0	0.0	0.0		1.0	Pass
2000 Hz	0.0	0.1	0.0		2.0	Pass
4000 Hz	0.0	0.0	0.0		3.0	Pass
8000 Hz	0.0	0.0	0.0		5.0	Pass
16000 Hz	-0.1	-0.1	-0.1		+5, -INF.	Pass

6. Frequency and time weightings at 1kHz

UUC Setting	STD REF	Measured		UNCERTAINTY ( $\pm$ dB)	Acceptance Limit ( $\pm$ dB)	Result
FAST / 37-139		UUC	ERR			
UUC Weighting	(dB)	(dB)	(dB)	0.20		
A	114.00	114.0	0.0			
C	114.00	114.0	0.0			
Z	114.00	114.0	0.0			

UUC Setting	STD REF	Measured		UNCERTAINTY ( $\pm$ dB)	Acceptance Limit ( $\pm$ dB)	Result
37-139 / A		UUC	ERR			
UUC Time Response	(dB)	(dB)	(dB)	0.20		
Fast	114.00	114.0	0.0			
Slow	114.00	114.0	0.0			
Leq	114.00	114.0	0.0			



Certificate No : 24-SLM-237

Request No : Req-2024-1456

### 7. Long Term Stability

UUC Setting	Measured	UNCERTAINTY	Acceptance	Result
FAST / A / 37-139	UUC		Limit	
STD Setting	(dB)	( ± dB)	( ± dB)	
Initial	114.0			
Final	114.0			
Deviated	0.0	0.10	0.30	Pass

### 8. Level linearity on the reference level range

UUC Setting	Anticipated	Deviation		UNCERTAINTY	Acceptance	Result
FAST / A / 37-139	REF	UUC	ERR		Limit	
STD dB	(dB)	(dB)	(dB)	( ± dB)	( ± dB)	
139.00	139	139.0	0.0	0.30	1.1	Pass
134.00	134	134.0	0.0		1.1	Pass
129.00	129	129.0	0.0		1.1	Pass
124.00	124	124.0	0.0		1.1	Pass
119.00	119	119.0	0.0		1.1	Pass
114.00	114	114.0	0.0		1.1	Pass
109.00	109	109.0	0.0		1.1	Pass
104.00	104	104.0	0.0		1.1	Pass
99.00	99	99.0	0.0		1.1	Pass
94.00	94	94.0	0.0		1.1	Pass
89.00	89	89.0	0.0		1.1	Pass
84.00	84	84.0	0.0		1.1	Pass
79.00	79	79.0	0.0		1.1	Pass
74.00	74	74.0	0.0		1.1	Pass
69.00	69	69.0	0.0		1.1	Pass
64.00	64	64.0	0.0		1.1	Pass
59.00	59	59.0	0.0		1.1	Pass
54.00	54	54.0	0.0		1.1	Pass
49.00	49	49.0	0.0		1.1	Pass
44.00	44	44.1	0.1		1.1	Pass
39.00	39	39.4	0.4		1.1	Pass
38.00	38	38.5	0.5		1.1	Pass



Certificate No : 24-SLM-237

Request No : Req-2024-1456

### 9. Level linearity including the level range control

UUC Setting	STD	Measured		UNCERTAINTY ( ± dB)	Acceptance Limit	Result
FAST / A	REF	UUC	ERR		( ± dB)	
UUC Range	(dB)	(dB)	(dB)		( ± dB)	
37-139	43.80	43.9	0.1	0.30	1.1	Pass
	114	114.0	0.0		1.1	Pass

### 10. Tone burst response

UUC Setting	STD	Anticipated	Measured		UNCERTAINTY ( ± dB)	Acceptance Limit	Result
A / 37-139	Toneburst	Ref	UUC	ERR		( ± dB)	
UUC Time Response	(ms)	(dB)	(dB)	(dB)		( ± dB)	
Fast	200	135.0	134.9	-0.1	0.20	1.0	Pass
	2	118.0	117.9	-0.1		+1.0, -2.5	Pass
	0.25	109.0	108.7	-0.3		+1.5, -5.0	Pass
Slow	200	128.6	128.4	-0.2		1.0	Pass
	2	109.0	108.8	-0.2		+1.0, -5.0	Pass
SEL	200	129.0	129.0	0.0		1.0	Pass
	2	109.0	109.1	+0.1		+1.0, -2.5	Pass
	0.25	100.0	99.9	-0.1		+1.5, -5.0	Pass

### 11. Peak C Sound level

UUC Setting	Anticipated	Measured		UNCERTAINTY ( ± dB)	Acceptance Limit	Result
FAST / C / 95-142	REF	UUC	ERR		( ± dB)	
STD Setting	(dB)	(dB)	(dB)		( ± dB)	
Complete cycle	137.4	136.8	-0.60	0.20	3.0	Pass
Positive half cycle	136.4	136.2	-0.20		2.0	Pass
Negative half cycle	136.4	136.2	-0.20		2.0	Pass

Certificate No : 24-SLM-237

Request No : Req-2024-1456

## 12. Overload indication

UUC Setting	Measured	UNCERTAINTY  ( ± dB)	Acceptance	Result
FAST / A / 37-139	UUC		Limit	
STD Setting	(dB)		( ± dB)	
Positive one-half cycle	142.6			
Negative one-half cycle	142.6			
Deviated	0.0	0.20	1.5	Pass

## 13. High Level Stability

UUC Setting	Measured	UNCERTAINTY  ( ± dB)	Acceptance	Result
FAST / A / 37-139	UUC		Limit	
STD Setting	(dB)		( ± dB)	
Initial	138.0			
Final	138.0			
Deviated	0.0	0.10	0.30	Pass

### Note :

Function	Maximum-permitted Uncertainty of measurement
1. Indication at the calibration check frequency	Not applicable
2. Self-generated noise, Microphone installed	Not applicable
3. Self-generated noise, Microphone replaced by the electrical input signal device	Not applicable
4. Acoustic signal test of frequency weightings at 10 Hz to 4 kHz	0.60 dB
4. Acoustic signal test of frequency weightings at >4 kHz to 10 kHz	0.70 dB
5. Electrical signal test of frequency weightings, Weighting network response with relative to 1 kHz	0.20 dB
6. Frequency and time weightings at 1kHz	0.20 dB
7. Long Term Stability	0.10 dB
8. Level linearity on the reference level range	0.30 dB
9. Level linearity including the level range control	0.30 dB
10. Tone burst response	0.30 dB
11. Peak C Sound level	0.35 dB
12. Overload indication	0.25 dB
13. High Level Stability	0.10 dB

- Acceptance limit and Maximum-permitted Uncertainty was IEC 61672-1:2013.

Certificate No : 24-SLM-237

Request No : Req-2024-1456

### Decision Rule for Statements of Conformity


The standard decision rule employed for the statements of conformity to each calibration result will be applied using ILAC-G8:09/2019; Guidelines on the Reporting of Compliance with Specification as following Fig. and statements

Pass = The measurement result plus the expanded uncertainty with a 95% coverage probability were within the limit.

Pass<sup>1</sup> = The measurement result was within the limit. However, a portion of the expanded uncertainty of measurement at 95% exceeds the limit.

Fail<sup>1</sup> = The measurement result was out of the limit. However, a portion of the expanded uncertainty of measurement at 95% is within the limit.

Fail = The measurement result plus the expanded uncertainty with a 95% coverage probability were outside the limit.

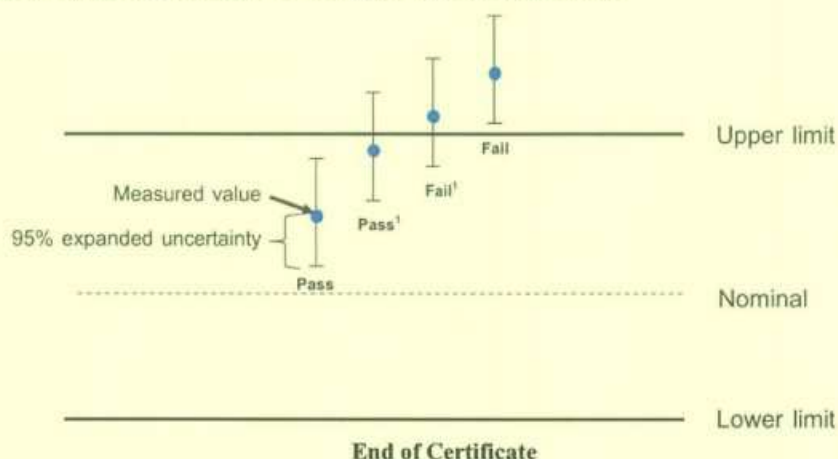



**ELECTRICAL AND ELECTRONICS INSTITUTE  
FOUNDATION FOR INDUSTRIAL DEVELOPMENT**

975 Moo 4, Bangpoo Industrial Estate, Soi 8, Sukhumvit Road km 37,

Phraek Sa, Mueang Samut Prakan, Samut Prakan 10280

Tel: +66 2709 4860 Fax: +66 2324 0917



Certificate No.: CP20240291EA

Operation No.: CP2024070254

## Certificate of Calibration

**Equipment:** Sound Level Meter

**Manufacturer:** Larson Davis (Meter), PCB (Microphone), PCB (Preamplifier)

**Model/Type:** LxT2 (Meter), 375A04B02 (Microphone), PRMLxT2C (Preamplifier)

**Serial No.:** 0005396 (Meter), 329350 (Microphone), 073805 (Preamplifier)

**ID No.:** UAE.EFM.033/2564

**Customer:** United Analyst and Engineering Consultant Co.,Ltd.

**Address:** 81 Soi Udomsuk 41, Sukhumvit Road, Bangchak  
Phrakhanong, Bangkok 10260

**Received Date:** 25 July 2024

**Calibrated Date:** 5 - 6 August 2024

**Issued Date:** 7 August 2024

**Calibrated by:** Ms. Juntaporn Kunhakom

Approved by:

( Mr. Sittichai Swaksuriyawong )

Group Manager

This report was prepared electronically using applicable electronic signature. Printing or copy of file are considered as a copy of the document.

The reported uncertainty of measurement was based on standard uncertainty multiplied by a coverage factor ( $k$ ) providing a level of confidence of approximately 95%. This certificate may not be reproduced other than in full except with the prior written approval of the Electrical and Electronics Institute, Foundation for Industrial Development.

Certificate No.: CP20240291EA

### Calibration Report

**Equipment:** Sound Level Meter  
**Manufacturer:** Larson Davis (Meter), PCB (Microphone), PCB (Preamplifier)  
**Model/Type:** LxT2 (Meter), 375A04B02 (Microphone), PRMLxT2C (Preamplifier)  
**Serial No.:** 0005396 (Meter), 329350 (Microphone), 073805 (Preamplifier)  
**ID No.:** UAE.EFM.033/2564  
**Ambient Temperature:** ( 23 ± 2 ) °C  
**Relative Humidity:** ( 50 ± 15 ) %  
**Pressure:** (101.3 ± 1.5) kPa  
**Method of Calibration :-**  
IEC 61672-3:2013.

#### Condition of this result of calibration

1. Reference standards instrument :-

Instrument	Model	Serial No.	Cert. No.	Due Date
1) Standard microphone	4180	2787490	AA-1012-23	12 November 2024
2) Arbitrary Function Generator	AFG2021	C010063	CK20240048EA	23 June 2025
3) Programmable Attenuator	PA5	2755	EF-0040-23	1 October 2024
4) 6.5 Digit precision multimeter	8846A	9610014	CB20230200EA	15 November 2024
5) Pressure humidity and Temperature Transmitter	PTU301	L3950483	CL1-P240023 CD20240142EA	24 March 2025 12 June 2025
6) Pressure humidity and Temperature Transmitter	PTU301	L3950484	CL1-P240030 CD20240143EA	11 April 2025 12 June 2025
7) Performance Audio Analyzer	U8903B	MY56510003	CB20240035EB CK20230072EA	13 February 2025 13 September 2024

2. This result of calibration was found accurate as shown on date and place of calibration only.

3. This certification is traceable to the international system of unit maintained at :-

Reference standards instrument for Acoustic function

- National Institute of Metrology (Thailand)

Reference standards instrument for Electrical function

- National Institute of Metrology (Thailand)

- Electrical and Electronics Institute; NSC Accredited Calibration No.0119

#### Result of Calibration:-

Function : 1. Indication at the calibration check frequency

Reference Acoustic Signal (dB)	Measured value (dB)	Deviation (dB)	Acceptance limits (dB)
-	-	-	-



Certificate No.: CP20240291EA

## Calibration Report

Function : 2. Self-generated Noise

### 2.1 Microphone Installed

Measured value (dB)
29.3

### 2.2 Microphone replaced by the electrical input signal device

Frequency Weighting	Measured value (dB)
A-weighting	29.1
C-weighting	28.8
Z-weighting	34.1

Function : 3. Acoustical signal tests of frequency weightings (Without Windscreen)

Meter free-field acoustic response at a level of 84 dB.

Frequency (Hz)	Deviation from various Frequency Weighting Response Curve			
	C-Weighting (dB)	A-Weighting (dB)	Z-Weighting (dB)	Acceptance limits (dB)
125	0.3	0.1	0.3	±1.5
1000	-0.1	-0.1	-0.1	±1.0
8000	0.2	0.2	0.2	±5.0

Function : 4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various Frequency Weighting Response Curve			
	C-Weighting (dB)	A-Weighting (dB)	Z-Weighting (dB)	Acceptance limits (dB)
63	0.0	0.0	0.0	±2.0
125	0.0	0.0	0.0	±1.5
250	0.0	0.0	0.0	±1.5
500	0.0	0.0	0.0	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.0	0.0	±2.0
4000	0.0	0.0	0.0	±3.0
8000	0.0	-0.1	0.0	±5.0

Function : 5. Frequency and time weighting at 1 kHz

### 5.1 Frequency weighting at 1 kHz

Frequency Weighting	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
C-weighting	94.0	0.0	±0.2
A-weighting	94.0	0.0	±0.2
Z-weighting	94.0	0.0	±0.2

Certificate No.: CP20240291EA

### Calibration Report

#### 5.2 Time weighting at 1 kHz

Time Weighting	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
Fast	94.0	0.0	±0.1
Slow	94.0	0.0	±0.1
LAeq	94.0	0.0	±0.1

#### Function : 6. Long-Term Stability

Long-term stability over 30 minutes, with steady 1 kHz signal at reference level.

Time Period to Apply Signal (min)	Reference SPL (dB)	Record SPL at Conclusion of Time Period (dB)	Deviated value (dB)	Acceptance limits (dB)
30	94.0	94.0	0.0	±0.3

#### Function : 7. Level Linearity on the reference level range

##### 7.1 Level Linearity on the reference level range, Upper

Anticipated Value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
94.0	94.0	0.0	±1.1
99.0	99.0	0.0	±1.1
104.0	104.0	0.0	±1.1
109.0	109.0	0.0	±1.1
114.0	114.0	0.0	±1.1
119.0	119.0	0.0	±1.1
124.0	124.0	0.0	±1.1
129.0	129.0	0.0	±1.1
134.0	134.1	0.1	±1.1
139.0	139.1	0.1	±1.1
140.0	140.1	0.1	±1.1
141.0	141.1	0.1	±1.1

Certificate No.: CP20240291EA

### Calibration Report

#### 7.2 Level Linearity on the reference level range, Lower

Anticipated Value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
94.0	94.0	0.0	±1.1
89.0	89.0	0.0	±1.1
84.0	84.0	0.0	±1.1
79.0	79.0	0.0	±1.1
74.0	74.0	0.0	±1.1
69.0	69.0	0.0	±1.1
64.0	64.0	0.0	±1.1
59.0	59.0	0.0	±1.1
54.0	54.0	0.0	±1.1
49.0	49.0	0.0	±1.1
44.0	44.1	0.1	±1.1
43.0	43.1	0.1	±1.1
42.0	42.2	0.2	±1.1
41.0	41.2	0.2	±1.1
40.0	40.3	0.3	±1.1

#### Function : 8. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
Fast	200	135.9	-0.1	±1.0
	2	118.8	-0.2	+1.0 ; -2.5
	0.25	109.8	-0.2	+1.5 ; -5.0
Slow	200	129.5	-0.1	±1.0
	2	109.9	-0.1	+1.0 ; -5.0
LAE	200	130.0	0.0	±1.0
	2	110.0	0.0	+1.0 ; -2.5
	0.25	101.0	0.0	+1.5 ; -5.0

#### Function : 9. Peak C sound level

Number of cycles in test signal	Anticipated Value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
Complete cycle	135.4	134.8	-0.6	±3.0
Positive half cycle	134.4	134.0	-0.4	±2.0
Negative half cycle	134.4	134.0	-0.4	±2.0

#### Function : 10. Overload indication

Measured value (dB)		Deviated value (dB)	Acceptance limits (dB)
Positive one-half cycle	Negative one-half cycle		
143.4	143.4	0.0	±1.5

เอกสารไม่ควบคุม

Certificate No.: CP20240291EA

### Calibration Report

Function : 11. High-Level Stability

High-level stability over 5 minutes, with steady 1 kHz signal, 1 dB below upper boundary.

Time Period to Apply Signal (min)	Reference SPL (dB)	Record SPL at Conclusion of Time Period (dB)	Deviated value (dB)	Acceptance limits (dB)
5	139.0	139.0	0.0	±0.3

### Uncertainty of measurement

Function	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1) Indication at the calibration check frequency	0.30	Not applicable
2) Self-generated Noise	0.10	Not applicable
3) Acoustical signal tests of frequency weightings - Free-field sound pressure response level	0.30	0.60 (10Hz to 4kHz) 0.70 (>4kHz to 10kHz)
4) Electrical signal tests of frequency weightings	0.20	0.20
5) Frequency and time weighting at 1 kHz	0.20	0.20
6) Long-Term Stability	0.10	0.10
7) Level Linearity on the reference level range	0.30	0.30
8) Tone burst response	0.20	0.30
9) Peak C sound level	0.20	0.35
10) Overload indication	0.20	0.25
11) High-Level Stability	0.10	0.10

- Remarks:
1. Indication at the calibration check frequency can not measured because customer does not provide a sound calibrator.
  2. The acceptance limit is for the deviated value.
  3. Acceptance limits was IEC61672-3:2013 Class 2.
  4. The coverage factor  $k = 2.00$

- - End of Report - -

## Certificate of Calibration

### Customer

Name : UNITED ANALYST AND ENGINEERING CONSULTANT CO., LTD.  
Address : 81 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Prakanong, Bangkok  
10260

Certificate No : 24-AFM-158

Request No : Req-2024-1574

### Unit Under Calibration Details

Measurement Item : Air Flow Meter  
Manufacturer : TSI Accuracy : 2% or 0.005 lpm, whichever is greater  
Model : 4146 Sensor Model : -  
Serial Number : 41462327003 Sensor Serial Number : -  
ID : UAE.EFM.126/2566 Instrument Status : Used  
Location of Calibration : LAB 4 AIR VELOCITY METER

### Calibration Environment and Details

Temperature : 23 °C ± 3 °C  
Humidity : 55 %RH ± 20 %RH  
Barometric Pressure : 1013 hPa ± 10 hPa  
Received Date : 15 July 2024  
Calibration Date : 19 August 2024  
Calibration Procedure : In-house method CP-AFM-01 by Comparison technique with Standard Primary Flow Calibrator


Reference Standard	Model	Serial Number	Traceble	Due Calibration
Air Flow Meter	Gilibrator 3 Low flow	18501010006	Sensidyne	6 August 2025
Air Flow Meter	Gilibrator 3 Standard flow	19031011003	Sensidyne	2 August 2025
Temperature meter	GT 11	08000057	Qreborn	1 March 2025
Pressure meter	CPG2400	41000KDU/651882	TPA	9 November 2024


### Traceability :

This Certificate is traceable to SI Unit through Sensidyne A2LA Accreditation No. 3943.01

### Note :

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor  $k = 2$ , providing a level of confidence approximately 95 %.

Calibration By :   
Mr. Noppadon Luangart  
Service Calibration Engineer

Approved By :   
Mr. Pacit Mathavorn  
Calibration Engineer Supervisor

Issue Date : 27 August 2024

**เอกสารไม่ควบคุม**



Certificate No : 24-AFM-158

Request No : Req-2024-1574

**Result of Calibration : Without Adjustment**

Temperature (°C)	Pressure (kPa)	STD (l/min)	UUC (l/min)	Error (l/min)	Uncertainty (l/min)	MPE (l/min)	Result
22.70	100.45	0.020	0.023	0.003	0.0013	0.005	N/A
22.60	100.51	0.050	0.054	0.004	0.0033	0.005	N/A
22.70	100.50	0.099	0.105	0.006	0.0028	0.005	N/A
22.70	100.49	0.200	0.215	0.015	0.0056	0.005	N/A
22.80	100.54	0.500	0.524	0.024	0.007	0.010	N/A
23.00	100.52	1.000	1.040	0.040	0.014	0.020	N/A
23.10	100.55	1.698	1.768	0.070	0.024	0.034	N/A
23.20	100.63	1.999	2.078	0.079	0.029	0.040	N/A
23.30	100.75	2.998	3.129	0.131	0.043	0.060	N/A
23.50	100.87	4.002	4.168	0.166	0.056	0.080	N/A
23.60	100.99	5.001	5.187	0.186	0.072	0.100	N/A

**Note**                      STD : Standard                      UUC : Unit Under Calibration  
 - UUC Reference Condition : 21.1 °C, 101.3 kPa, Air  
 - Flow Rate was corrected for non-standard operating condition by using equation :

$$Q_{meas} = Q_{ref} \times \frac{P_{ref}}{P_{meas}} \times \frac{T_{meas}}{T_{ref}}$$

where    Q = Flow Rate                      P = Absolute Pressure                      T = Absolute Temperature  
             Meas = Measurement Condition                      ref = Standard Condition

\* Indicates non accredited

MPE = Maximum Permissible Error (Specified in Manufacturer's Specifications)

N/A = Not Available, Customer does not require a statement of conformity.

**เอกสารไม่ควบคุม**

Certificate No : 24-AFM-158

Request No : Req-2024-1574

### Decision Rule for Statements of Conformity


The standard decision rule employed for the statements of conformity to each calibration result will be applied using ILAC-G8:09/2019: Guidelines on the Reporting of Compliance with Specification as following Fig. and statements

Pass = The measurement result plus the expanded uncertainty with a 95% coverage probability were within the limit.

Pass<sup>1</sup> = The measurement result was within the limit. However, a portion of the expanded uncertainty of measurement at 95% exceeds the limit.

Fail<sup>1</sup> = The measurement result was out of the limit. However, a portion of the expanded uncertainty of measurement at 95% is within the limit.

Fail = The measurement result plus the expanded uncertainty with a 95% coverage probability were outside the limit.

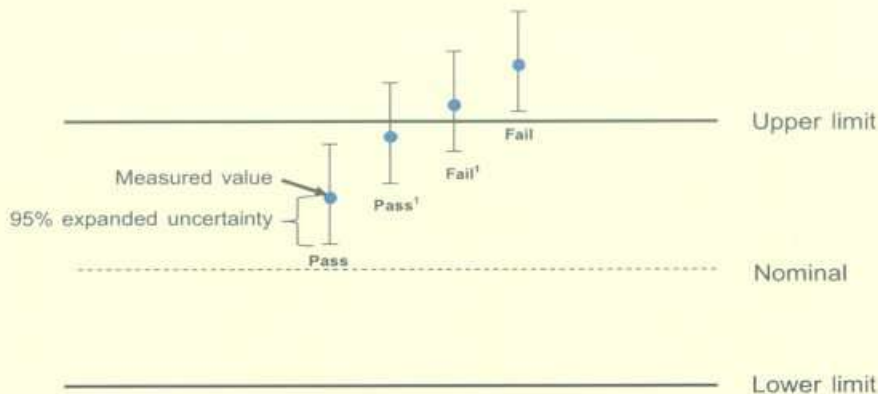

End of Certificate

เอกสารไม่ควบคุม

## Certificate of Calibration

### Customer

Name : UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.  
Address : 81 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Prakanong, Bangkok  
10260

Certificate No : 24-ASP-127

Request No : Req-2024-1791

### Unit Under Calibration Details

Measurement Item : Air Sampling Pump  
Manufacturer : SENSIDYNE  
Model : GilAir Plus  
Serial Number : 20230610196  
ID : UAE.EFM.127/2566  
Location of Calibration : LAB 4 AIR VELOCITY METER

Instrument Status : Used

### Calibration Environment and Details

Temperature :  $23^{\circ}\text{C} \pm 3^{\circ}\text{C}$   
Humidity :  $55\% \text{RH} \pm 20\% \text{RH}$   
Barometric Pressure :  $1013 \text{ hPa} \pm 10 \text{ hPa}$   
Received Date : 15 August 2024  
Calibration Date : 27 August 2024  
Calibration Procedure : In-house method CP-ASP-01 based on ISO 13137 by Comparison With Standard Air Flow Meter


Reference Standard	Model	Serial Number	Traceble	Due Calibration
Air Flow Meter	Gilibrator 3 Standard flow	19031011003	Sensidyne	2 August 2025
Digital Thermometer with Probe	GT11	08000057	Q.Reborn	1 March 2025
Barometer	CPG2400	41000KDU/651882	TPA	9 November 2024


### Traceability :

This Certificate is traceable to SI Unit through Sensidyne A2LA Accreditation No. 3943.01

### Note :

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor  $k = 2$ , providing a level of confidence approximately 95 %.

Calibration By :   
Mr. Noppadon Luangart  
Service Calibration Engineer

Approved By :   
Mr. Pacit Mathavorn  
Calibration Engineer Supervisor

Issue Date : 27 August 2024

**เอกสารไม่ควบคุม**

Certificate No : 24-ASP-127

Request No : Req-2024-1791

Result of Calibration : Low (Without Adjustment)

Temperature (°C)	Pressure (kPa)	STD (l/min)	UUC (l/min)	Error (l/min)	Error (l/min), (%)	MPE (l/min), (%)	**Back Pressure (inH <sub>2</sub> O)	Uncertainty (l/min)	Result
23.70	99.30	0.020	0.020	0.000	0 l/min	0.003 l/min	5	0.0011	Pass
23.70	95.65	0.022	0.020	-0.002	-0.002 l/min	0.003 l/min	20	0.0012	Pass1
23.70	90.21	0.017	0.020	0.003	0.003 l/min	0.003 l/min	40	0.0009	Pass1
23.80	99.20	0.051	0.050	-0.001	-0.001 l/min	0.003 l/min	5	0.0028	Pass1
23.80	95.43	0.051	0.050	-0.001	-0.001 l/min	0.003 l/min	20	0.0028	Pass1
23.80	90.86	0.049	0.050	0.001	0.001 l/min	0.003 l/min	40	0.0027	Pass1
23.70	99.11	0.101	0.100	-0.001	-1 (%)	5 (%)	5	0.0026	Pass
23.70	95.17	0.099	0.100	0.001	1 (%)	5 (%)	20	0.0026	Pass
23.70	90.02	0.096	0.100	0.004	4.2 (%)	5 (%)	40	0.0025	Pass1
23.70	99.11	0.201	0.200	-0.001	-0.5 (%)	5 (%)	5	0.0036	Pass
23.70	95.44	0.199	0.200	0.001	0.5 (%)	5 (%)	20	0.0036	Pass
23.70	90.47	0.195	0.200	0.005	2.6 (%)	5 (%)	40	0.0035	Pass

เอกสารไม่ควบคุม



Certificate No : 24-ASP-127

Request No : Req-2024-1791

**Result of Calibration : High(Without Adjustment)**

Temperature (°C)	Pressure (kPa)	STD (l/min)	UUC (l/min)	Error (l/min)	Error (l/min), (%)	MPE (l/min), (%)	**Back Pressure (inH <sub>2</sub> O)	Uncertainty (l/min)	Result
23.70	99.23	0.502	0.500	-0.002	-0.4 %	5 (%)	5	0.0080	Pass
23.70	95.63	0.509	0.500	-0.009	-1.8 %	5 (%)	20	0.0081	Pass
23.70	91.64	0.502	0.500	-0.002	-0.4 %	5 (%)	40	0.0080	Pass
23.70	99.10	1.003	1.000	-0.003	-0.3 (%)	5 (%)	5	0.016	Pass
23.70	95.30	0.996	1.000	0.004	0.4 (%)	5 (%)	20	0.016	Pass
23.70	91.43	0.988	1.000	0.012	1.2 (%)	5 (%)	35	0.016	Pass
23.70	99.06	1.711	1.700	-0.011	-0.6 (%)	5 (%)	5	0.027	Pass
23.70	95.22	1.674	1.700	0.026	1.6 (%)	5 (%)	20	0.027	Pass
23.70	92.85	1.659	1.700	0.041	2.5 (%)	5 (%)	30	0.027	Pass
23.70	99.11	2.005	2.000	-0.005	-0.2 (%)	5 (%)	5	0.032	Pass
23.70	95.26	1.968	2.000	0.032	1.6 (%)	5 (%)	20	0.032	Pass
23.70	92.71	1.953	2.000	0.047	2.4 (%)	5 (%)	30	0.031	Pass
23.60	99.07	3.012	3.000	-0.012	-0.4 (%)	5 (%)	5	0.048	Pass
23.60	95.10	2.992	3.000	0.008	0.3 (%)	5 (%)	20	0.048	Pass
23.60	92.74	2.980	3.000	0.020	0.7 (%)	5 (%)	30	0.048	Pass
23.60	99.03	4.005	4.000	-0.005	-0.1 (%)	5 (%)	5	0.064	Pass
23.60	97.72	4.007	4.000	-0.007	-0.2 (%)	5 (%)	10	0.064	Pass
23.60	95.14	4.007	4.000	-0.007	-0.2 %	5 (%)	20	0.064	Pass
23.60	99.00	5.004	5.000	-0.004	-0.1 %	5 (%)	5	0.080	Pass
23.60	97.25	5.009	5.000	-0.009	-0.2 %	5 (%)	12	0.080	Pass

**Note**

STD : Standard UUC : Unit Under Calibration

- UUC Reference Condition : At 25 °C, 101.3 kPa, Air

- Flow Rate was corrected for non-standard operating condition by using equation :

$$Q_{\text{meas}} = Q_{\text{ref}} \times \frac{P_{\text{ref}}}{P_{\text{meas}}} \times \frac{T_{\text{meas}}}{T_{\text{ref}}}$$

where Q = Flow Rate P = Absolute Pressure T = Absolute Temperature  
 meas = Measurement Condition ref = Standard Condition

**เอกสารไม่ควบคุม**



Certificate No : 24-ASP-127

Request No : Req-2024-1791

#### Note

\* Indicates non accredited

\*\* Specified in ISO 13137, Back Pressure control  $\pm 1$  inH2O

MPE = Maximum Permissible Error (Specified in Manufacturer's Specification)

#### Decision Rule for Statements of Conformity


The standard decision rule employed for the statements of conformity to each calibration result will be applied using ILAC-G8:09/2019: Guidelines on the Reporting of Compliance with Specification as following Fig. and statements

Pass = The measurement result plus the expanded uncertainty with a 95% coverage probability were within the limit.

Pass<sup>1</sup> = The measurement result was within the limit. However, a portion of the expanded uncertainty of measurement at 95% exceeds the limit.

Fail<sup>1</sup> = The measurement result was out of the limit. However, a portion of the expanded uncertainty of measurement at 95% is within the limit.

Fail = The measurement result plus the expanded uncertainty with a 95% coverage probability were outside the limit.

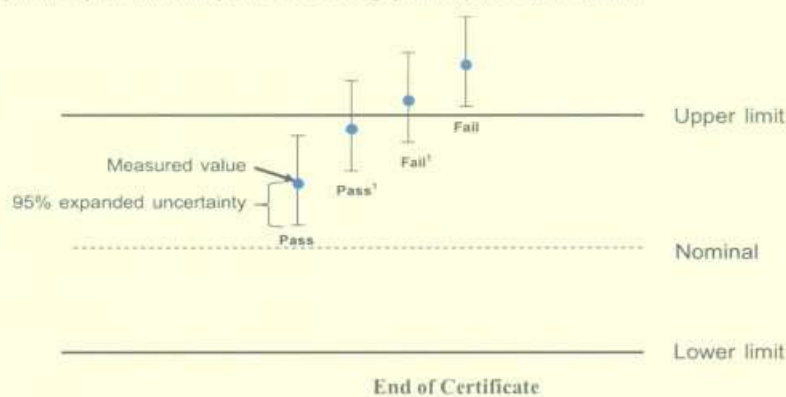

**เอกสารไม่ควบคุม**

## Certificate of Calibration

### Customer

Name : UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.  
Address : 81 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Prakanong, Bangkok 10260

Certificate No : 24-ASP-048

Request No : Req-2024-0817

### Unit Under Calibration Details

Measurement Item : Air Sampling Pump  
Manufacturer : SENSIDYNE  
Model : GilAir Plus  
Serial Number : 20230410024  
ID : UAE.EFM.093/2566  
Location of Calibration : LAB 4 AIR VELOCITY METER

### Calibration Environment and Details

Temperature :  $23^{\circ}\text{C} \pm 3^{\circ}\text{C}$   
Humidity :  $55\% \text{RH} \pm 20\% \text{RH}$   
Barometric Pressure :  $1013 \text{ hPa} \pm 10 \text{ hPa}$   
Received Date : 10 April 2024  
Calibration Date : 8 May 2024  
Calibration Procedure : In-house method CP-ASP-01 based on ISO 13137 by Comparison With Standard Air Flow Meter


Reference Standard	Model	Serial Number	Traceble	Due Calibration
Air Flow Meter	Gilibrator 3 Low flow	18501010006	Sensidyne	12 July 2024
Air Flow Meter	Gilibrator 3 Standard flow	19031011003	Sensidyne	12 July 2024
Digital Thermometer with Probe	GT11	12000077	Q.Reborn	27 October 2024
Barometer	CPG2400	41000KDU/651882	TPA	9 November 2024


### Traceability :

This Certificate is traceable to SI Unit through Sensidyne A2LA Accreditation No. 3943.01

### Note :

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor  $k = 2$ , providing a level of confidence approximately 95%.

Calibration By :   
Mr. Noppadon Luangart  
Service Calibration Engineer

Approved By :   
Mr. Pacit Mathavorn  
Calibration Engineer Supervisor

Issue Date : 8 May 2024

**เอกสารไม่ควบคุม**

Certificate No : 24-ASP-048

Request No : Req-2024-0817

Result of Calibration : Low

Temperature (°C)	Pressure (kPa)	STD (l/min)	UUC (l/min)	Error (l/min)	Error (l/min), (%)	**Allowable Range (l/min), (%)	***Back Pressure (inH <sub>2</sub> O)	Uncertainty (l/min)
24.40	99.51	0.021	0.020	-0.001	-0.001 l/min	0.003 l/min	5	0.0009
24.40	95.59	0.021	0.020	-0.001	-0.001 l/min	0.003 l/min	20	0.0009
24.40	90.62	0.019	0.020	0.001	0.001 l/min	0.003 l/min	40	0.0009
24.50	99.31	0.050	0.050	0.000	0 l/min	0.003 l/min	5	0.0012
24.50	95.37	0.050	0.050	0.000	0 l/min	0.003 l/min	20	0.0012
24.50	90.84	0.051	0.050	-0.001	-0.001 l/min	0.003 l/min	40	0.0012
24.30	99.32	0.100	0.100	0.000	0 %	5 %	5	0.0018
24.30	95.56	0.098	0.100	0.002	2 %	5 %	20	0.0018
24.30	90.64	0.099	0.100	0.001	1 %	5 %	40	0.0018
24.60	99.36	0.200	0.200	0.000	0 %	5 %	5	0.0033
24.60	95.31	0.199	0.200	0.001	0.5 %	5 %	20	0.0033
24.60	90.25	0.198	0.200	0.002	1 %	5 %	40	0.0033

เอกสารไม่ควบคุม

Certificate No : 24-ASP-048

Request No : Req-2024-0817

Result of Calibration : High

Temperature (°C)	Pressure (kPa)	STD (l/min)	UUC (l/min)	Error (l/min)	Error (l/min), (%)	**Allowable Range (l/min), (%)	***Back Pressure (inH <sub>2</sub> O)	Uncertainty (l/min)
24.60	99.27	0.502	0.500	-0.002	-0.4 %	5 %	5	0.008
24.60	95.45	0.508	0.500	-0.008	-1.6 %	5 %	20	0.009
24.60	90.67	0.505	0.500	-0.005	-1 %	5 %	40	0.008
25.00	99.26	1.010	1.000	-0.010	-1 %	5%	5	0.015
25.00	95.37	1.003	1.000	-0.003	-0.3 %	5%	20	0.015
25.00	90.43	0.989	1.000	0.011	1.1 %	5%	40	0.015
25.00	99.24	1.711	1.700	-0.011	-0.6 %	5%	5	0.027
25.00	95.51	1.665	1.700	0.035	2.1 %	5%	20	0.027
25.00	91.98	1.654	1.700	0.046	2.8 %	5%	35	0.029
24.80	99.30	2.007	2.000	-0.007	-0.3 %	5%	5	0.032
24.80	96.75	1.978	2.000	0.022	1.1 %	5%	15	0.032
24.80	92.88	1.969	2.000	0.031	1.6 %	5%	30	0.032
25.10	99.28	3.010	3.000	-0.010	-0.3 %	5%	5	0.048
25.10	96.75	3.005	3.000	-0.005	-0.2 %	5%	15	0.048
25.10	92.86	2.992	3.000	0.008	0.3 %	5%	30	0.048
25.00	99.26	4.003	4.000	-0.003	-0.1 %	5%	5	0.064
25.00	98.01	4.015	4.000	-0.015	-0.4 %	5%	10	0.064
25.00	95.39	4.011	4.000	-0.011	-0.3 %	5%	20	0.064
25.00	99.20	5.008	5.000	-0.008	-0.2 %	5%	5	0.079
25.00	97.94	4.998	5.000	0.002	0 %	5%	10	0.079

Note STD : Standard UUC : Unit Under Calibration

- UUC Reference Condition : At 25 °C, 101.3 kPa, Air

- Flow Rate was corrected for non-standard operating condition by using equation :

$$Q_{meas} = Q_{ref} \times \frac{P_{ref}}{P_{meas}} \times \frac{T_{meas}}{T_{ref}}$$

where Q = Flow Rate P = Absolute Pressure T = Absolute Temperature

Meas = Measurement Condition ref = Standard Condition

Note

\* Indicates non accredited

\*\* Reference Specifications : ± 5% of set flow or ±3 cc/min whichever is higher

\*\*\* Specified in ISO 13137, Back Pressure control ± 1 inH<sub>2</sub>O

End of Certificate

เอกสารไม่ควบคุม



## Certificate of Calibration

### Customer

Name : UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.  
Address : 81 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Prakanong, Bangkok 10260

Certificate No : 24-ASP-041

Request No : Req-2024-0818

### Unit Under Calibration Details

Measurement Item : Air Sampling Pump  
Manufacturer : SENSIDYNE  
Model : GilAir Plus  
Serial Number : 20230410025  
ID : UAE.EFM.094/2566  
Location of Calibration : LAB 4 AIR VELOCITY METER

### Calibration Environment and Details

Temperature :  $23^{\circ}\text{C} \pm 3^{\circ}\text{C}$   
Humidity :  $55\% \text{RH} \pm 20\% \text{RH}$   
Barometric Pressure :  $1013 \text{ hPa} \pm 10 \text{ hPa}$   
Received Date : 10 April 2024  
Calibration Date : 6 May 2024  
Calibration Procedure : In-house method CP-ASP-01 based on ISO 13137 by Comparison With Standard Air Flow Meter


Reference Standard	Model	Serial Number	Traceble	Due Calibration
Air Flow Meter	Gilibrator 3 Low flow	18501010006	Sensidyne	12 July 2024
Air Flow Meter	Gilibrator 3 Standard flow	19031011003	Sensidyne	12 July 2024
Digital Thermometer with Probe	GT11	12000077	Q.Reborn	27 October 2024
Barometer	CPG2400	41000KDU/651882	TPA	9 November 2024


### Traceability :

This Certificate is traceable to SI Unit through Sensidyne A2LA Accreditation No. 3943.01

### Note :

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor  $k = 2$ , providing a level of confidence approximately 95 %.

Calibration By :   
Mr. Noppadon Luangart  
Service Calibration Engineer

Approved By :   
Mr. Pacit Mathavorn  
Calibration Engineer Supervisor

Issue Date : 6 May 2024

**เอกสารไม่ควบคุม**



Certificate No : 24-ASP-041

Request No : Req-2024-0818

Result of Calibration : Low

Temperature (°C)	Pressure (kPa)	STD (l/min)	UUC (l/min)	Error (l/min)	Error (l/min), (%)	**Allowable Range (l/min), (%)	***Back Pressure (inH <sub>2</sub> O)	Uncertainty (l/min)
25.00	99.53	0.020	0.020	0.000	0 l/min	0.003 l/min	5	0.0009
25.00	95.67	0.019	0.020	0.001	0.001 l/min	0.003 l/min	20	0.0009
25.00	90.93	0.018	0.020	0.002	0.002 l/min	0.003 l/min	40	0.0009
24.80	99.53	0.049	0.050	0.001	0.001 l/min	0.003 l/min	5	0.0012
24.80	95.93	0.049	0.050	0.001	0.001 l/min	0.003 l/min	20	0.0012
24.80	90.50	0.048	0.050	0.002	0.002 l/min	0.003 l/min	40	0.0012
25.00	99.52	0.100	0.100	0.000	0 %	5 %	5	0.0018
25.00	95.68	0.097	0.100	0.003	3.1 %	5 %	20	0.0018
25.00	90.60	0.096	0.100	0.004	4.2 %	5 %	40	0.0018
24.90	99.55	0.201	0.200	-0.001	-0.5 %	5 %	5	0.0033
24.90	95.70	0.199	0.200	0.001	0.5 %	5 %	20	0.0033
24.90	90.90	0.198	0.200	0.002	1 %	5 %	40	0.0033

**เอกสารไม่ควบคุม**

Certificate No : 24-ASP-041

Request No : Req-2024-0818

Result of Calibration : High

Temperature (°C)	Pressure (kPa)	STD (l/min)	UUC (l/min)	Error (l/min)	Error (l/min), (%)	**Allowable Range (l/min), (%)	***Back Pressure (inH <sub>2</sub> O)	Uncertainty (l/min)
24.90	99.56	0.501	0.500	-0.001	-0.2 %	5 %	5	0.008
24.90	95.75	0.506	0.500	-0.006	-1.2 %	5 %	20	0.008
24.90	90.78	0.498	0.500	0.002	0.4 %	5 %	40	0.008
25.00	99.53	1.008	1.000	-0.008	-0.8 %	5%	5	0.015
25.00	95.76	0.996	1.000	0.004	0.4 %	5%	20	0.015
25.00	90.42	0.972	1.000	0.028	2.9 %	5%	40	0.015
24.80	99.54	1.713	1.700	-0.013	-0.8 %	5%	5	0.027
24.80	95.62	1.656	1.700	0.044	2.7 %	5%	20	0.027
24.80	92.09	1.627	1.700	0.073	4.5 %	5%	35	0.027
24.90	99.52	2.005	2.000	-0.005	-0.2 %	5%	5	0.032
24.90	96.90	1.960	2.000	0.040	2 %	5%	15	0.032
24.90	93.24	1.929	2.000	0.071	3.7 %	5%	30	0.032
24.90	99.49	3.015	3.000	-0.015	-0.5 %	5%	5	0.048
24.90	96.95	2.999	3.000	0.001	0 %	5%	15	0.048
24.90	93.23	2.986	3.000	0.014	0.5 %	5%	30	0.048
25.00	99.48	3.996	4.000	0.004	0.1 %	5%	5	0.064
25.00	98.19	4.006	4.000	-0.006	-0.1 %	5%	10	0.064
25.00	95.80	3.999	4.000	0.001	0 %	5%	20	0.064
24.90	99.44	5.012	5.000	-0.012	-0.2 %	5%	5	0.079
24.90	98.14	5.004	5.000	-0.004	-0.1 %	5%	10	0.079

Note

STD : Standard UUC : Unit Under Calibration

- UUC Reference Condition : At 25 °C, 101.3 kPa, Air

- Flow Rate was corrected for non-standard operating condition by using equation :

$$Q_{\text{meas}} = Q_{\text{ref}} \times \frac{P_{\text{ref}}}{P_{\text{meas}}} \times \frac{T_{\text{meas}}}{T_{\text{ref}}}$$

where Q = Flow Rate P = Absolute Pressure T = Absolute Temperature

Meas = Measurement Condition ref = Standard Condition

Note

\* Indicates non accredited

\*\* Reference Specifications ± 5% of set flow or ± 3 cc/min whichever is higher

\*\*\* Specified in ISO 13137, Back Pressure control ± 1 inH<sub>2</sub>O

End of Certificate

เอกสารไม่ควบคุม

## Certificate of Calibration

### Customer

Name : UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.  
Address : 81 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Prakanong, Bangkok 10260

Certificate No : 24-ASP-040

Request No : Req-2024-0820

### Unit Under Calibration Details

Measurement Item : Air Sampling Pump  
Manufacturer : SENSIDYNE  
Model : GilAir Plus  
Serial Number : 20230410027  
ID : UAE.EFM.096/2566  
Location of Calibration : LAB 4 AIR VELOCITY METER

### Calibration Environment and Details

Temperature :  $23^{\circ}\text{C} \pm 3^{\circ}\text{C}$   
Humidity :  $55\% \text{RH} \pm 20\% \text{RH}$   
Barometric Pressure :  $1013 \text{ hPa} \pm 10 \text{ hPa}$   
Received Date : 10 April 2024  
Calibration Date : 3 May 2024  
Calibration Procedure : In-house method CP-ASP-01 based on ISO 13137 by Comparison With Standard Air Flow Meter


Reference Standard	Model	Serial Number	Traceble	Due Calibration
Air Flow Meter	Gilibrator 3 Low flow	18501010006	Sensidyne	12 July 2024
Air Flow Meter	Gilibrator 3 Standard flow	19031011003	Sensidyne	12 July 2024
Digital Thermometer with Probe	GT11	12000077	Q.Reborn	27 October 2024
Barometer	CPG2400	41000KDU/651882	TPA	9 November 2024


### Traceability :

This Certificate is traceable to SI Unit through Sensidyne A2LA Accreditation No. 3943.01

### Note :

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor  $k = 2$ , providing a level of confidence approximately 95 %.

Calibration By :   
Mr. Noppadon Luangart  
Service Calibration Engineer

Approved By :   
Mr. Pacit Mathavorn  
Calibration Engineer Supervisor

Issue Date : 3 May 2024

**เอกสารไม่ควบคุม**

Certificate No : 24-ASP-040

Request No : Req-2024-0820

Result of Calibration : Low

Temperature (°C)	Pressure (kPa)	STD (l/min)	UUC (l/min)	Error (l/min)	Error (l/min), (%)	**Allowable Range (l/min), (%)	***Back Pressure (in H <sub>2</sub> O)	Uncertainty (l/min)
25.00	99.13	0.019	0.020	0.001	0.001 l/min	0.003 l/min	5	0.0009
25.00	95.28	0.022	0.020	-0.002	-0.002 l/min	0.003 l/min	20	0.0009
25.00	90.08	0.019	0.020	0.001	0.001 l/min	0.003 l/min	40	0.0009
24.80	98.92	0.050	0.050	0.000	0 l/min	0.003 l/min	5	0.0012
24.80	95.33	0.051	0.050	-0.001	-0.001 l/min	0.003 l/min	20	0.0012
24.80	90.37	0.052	0.050	-0.002	-0.002 l/min	0.003 l/min	40	0.0012
25.00	99.04	0.099	0.100	0.001	1 %	5 %	5	0.0018
25.00	95.23	0.099	0.100	0.001	1 %	5 %	20	0.0018
25.00	90.40	0.098	0.100	0.002	2 %	5 %	40	0.0018
24.90	99.11	0.201	0.200	-0.001	-0.5 %	5 %	5	0.0033
24.90	95.28	0.197	0.200	0.003	1.5 %	5 %	20	0.0033
24.90	90.20	0.197	0.200	0.003	1.5 %	5 %	40	0.0033

เอกสารไม่ควบคุม



Certificate No : 24-ASP-040

Request No : Req-2024-0820

Result of Calibration : High

Temperature (°C)	Pressure (kPa)	STD (l/min)	UUC (l/min)	Error (l/min)	Error (l/min), (%)	**Allowable Range (l/min), (%)	***Back Pressure (inH <sub>2</sub> O)	Uncertainty (l/min)
24.90	99.05	0.500	0.500	0.000	0 %	5 %	5	0.008
24.90	95.36	0.512	0.500	-0.012	-2.3 %	5 %	20	0.008
24.90	90.38	0.506	0.500	-0.006	-1.2 %	5 %	40	0.008
25.00	99.03	1.010	1.000	-0.010	-1 %	5%	5	0.015
25.00	95.19	1.003	1.000	-0.003	-0.3 %	5%	20	0.015
25.00	90.36	0.999	1.000	0.001	0.1 %	5%	40	0.015
24.80	99.02	1.711	1.700	-0.011	-0.6 %	5%	5	0.027
24.80	95.22	1.683	1.700	0.017	1 %	5%	20	0.027
24.80	91.52	1.666	1.700	0.034	2 %	5%	35	0.027
24.90	99.08	2.006	2.000	-0.006	-0.3 %	5%	5	0.032
24.90	96.51	1.988	2.000	0.012	0.6 %	5%	15	0.032
24.90	92.74	1.962	2.000	0.038	1.9 %	5%	30	0.032
24.90	99.01	3.012	3.000	-0.012	-0.4 %	5%	5	0.048
24.90	96.51	2.996	3.000	0.004	0.1 %	5%	15	0.048
24.90	92.77	2.974	3.000	0.026	0.9 %	5%	30	0.048
25.00	99.02	3.997	4.000	0.003	0.1 %	5%	5	0.064
25.00	97.69	3.990	4.000	0.010	0.3 %	5%	10	0.063
25.00	95.17	3.995	4.000	0.005	0.1 %	5%	20	0.064
24.90	99.01	5.006	5.000	-0.006	-0.1 %	5%	5	0.079
24.90	97.66	5.004	5.000	-0.004	-0.1 %	5%	10	0.079

Note STD : Standard UUC : Unit Under Calibration

- UUC Reference Condition : At 25 °C, 101.3 kPa, Air

- Flow Rate was corrected for non-standard operating condition by using equation :

$$Q_{\text{meas}} = Q_{\text{ref}} \times \frac{P_{\text{ref}}}{P_{\text{meas}}} \times \frac{T_{\text{meas}}}{T_{\text{ref}}}$$

where Q = Flow Rate P = Absolute Pressure T = Absolute Temperature

Meas = Measurement Condition ref = Standard Condition

Note

\* Indicates non accredited

\*\* Reference Specifications ± 5% of set flow or ±3 cc/min whichever is higher

\*\*\* Specified in ISO 13137, Back Pressure control ± 1 inH<sub>2</sub>O

End of Certificate

**เอกสารไม่ควบคุม**

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

FM-708-AFM-01 Rev.00 Issue date 01/07/19



## Certificate of Calibration

### Customer

Name : UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.  
Address : 81 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Prakanong, Bangkok 10260

Certificate No : 24-ASP-045

Request No : Req-2024-0814

### Unit Under Calibration Details

Measurement Item : Air Sampling Pump  
Manufacturer : SENSIDYNE  
Model : GilAir Plus  
Serial Number : 20230410021  
ID : UAE.EFM.090/2566  
Location of Calibration : LAB 4 AIR VELOCITY METER

### Calibration Environment and Details

Temperature : 23 °C ± 3 °C  
Humidity : 55 %RH ± 20 %RH  
Barometric Pressure : 1013 hPa ± 10 hPa  
Received Date : 10 April 2024  
Calibration Date : 7 May 2024  
Calibration Procedure : In-house method CP-ASP-01 based on ISO 13137 by Comparison With Standard Air Flow Meter


Reference Standard	Model	Serial Number	Traceble	Due Calibration
Air Flow Meter	Gilibrator 3 Low flow	18501010006	Sensidyne	12 July 2024
Air Flow Meter	Gilibrator 3 Standard flow	19031011003	Sensidyne	12 July 2024
Digital Thermometer with Probe	GT11	12000077	Q.Reborn	27 October 2024
Barometer	CPG2400	41000KDU/651882	TPA	9 November 2024


### Traceability :

This Certificate is traceable to SI Unit through Sensidyne A2LA Accreditation No. 3943.01

### Note :

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor  $k = 2$ , providing a level of confidence approximately 95 %.

Calibration By :   
Mr. Noppadon Luangart  
Service Calibration Engineer

Approved By :   
Mr. Pacit Mathavorn  
Calibration Engineer Supervisor

Issue Date : 7 May 2024

**เอกสารไม่ควบคุม**

Certificate No : 24-ASP-045

Request No : Req-2024-0814

Result of Calibration : Low

Temperature (°C)	Pressure (kPa)	STD (l/min)	UUC (l/min)	Error (l/min)	Error (l/min), (%)	**Allowable Range (l/min), (%)	***Back Pressure (inH <sub>2</sub> O)	Uncertainty (l/min)
24.40	99.81	0.020	0.020	0.000	0 l/min	0.003 l/min	5	0.0009
24.40	96.14	0.022	0.020	-0.002	-0.002 l/min	0.003 l/min	20	0.0009
24.40	91.07	0.021	0.020	-0.001	-0.001 l/min	0.003 l/min	40	0.0009
24.80	99.72	0.050	0.050	0.000	0 l/min	0.003 l/min	5	0.0012
24.80	96.13	0.051	0.050	-0.001	-0.001 l/min	0.003 l/min	20	0.0012
24.80	91.01	0.049	0.050	0.001	0.001 l/min	0.003 l/min	40	0.0012
24.80	99.73	0.100	0.100	0.000	0 %	5 %	5	0.0018
24.80	96.03	0.099	0.100	0.001	1 %	5 %	20	0.0018
24.80	91.11	0.097	0.100	0.003	3.1 %	5 %	40	0.0018
24.70	99.73	0.200	0.200	0.000	0 %	5 %	5	0.0033
24.70	96.08	0.198	0.200	0.002	1 %	5 %	20	0.0033
24.70	91.05	0.197	0.200	0.003	1.5 %	5 %	40	0.0033

**เอกสารไม่ควบคุม**

Certificate No : 24-ASP-045

Request No : Req-2024-0814

**Result of Calibration : High**

Temperature (°C)	Pressure (kPa)	STD (l/min)	UUC (l/min)	Error (l/min)	Error (l/min), (%)	**Allowable Range (l/min), (%)	***Back Pressure (inH <sub>2</sub> O)	Uncertainty (l/min)
24.90	99.70	0.500	0.500	0.000	0 %	5 %	5	0.008
24.90	95.81	0.509	0.500	-0.009	-1.8 %	5 %	20	0.008
24.90	91.16	0.506	0.500	-0.006	-1.2 %	5 %	40	0.008
25.00	99.80	1.009	1.000	-0.009	-0.9 %	5%	5	0.015
25.00	95.93	0.990	1.000	0.010	1 %	5%	20	0.015
25.00	91.12	0.972	1.000	0.028	2.9 %	5%	40	0.015
25.10	99.77	1.732	1.700	-0.032	-1.8 %	5%	5	0.027
25.10	95.95	1.644	1.700	0.056	3.4 %	5%	20	0.027
25.10	92.16	1.622	1.700	0.078	4.8 %	5%	35	0.027
24.80	99.74	2.002	2.000	-0.002	-0.1 %	5%	5	0.032
24.80	97.23	1.965	2.000	0.035	1.8 %	5%	15	0.032
24.80	93.49	1.939	2.000	0.061	3.1 %	5%	30	0.032
24.50	99.70	3.010	3.000	-0.010	-0.3 %	5%	5	0.048
24.50	97.13	2.977	3.000	0.023	0.8 %	5%	15	0.048
24.50	93.34	2.967	3.000	0.033	1.1 %	5%	30	0.048
25.00	99.65	4.003	4.000	-0.003	-0.1 %	5%	5	0.064
25.00	98.37	4.000	4.000	0.000	0 %	5%	10	0.064
25.00	95.81	4.001	4.000	-0.001	0 %	5%	20	0.064
24.30	99.61	5.013	5.000	-0.013	-0.3 %	5%	5	0.079
24.30	98.31	4.998	5.000	0.002	0 %	5%	10	0.079

**Note** STD : Standard UUC : Unit Under Calibration

- UUC Reference Condition : At 25 °C, 101.3 kPa, Air

- Flow Rate was corrected for non-standard operating condition by using equation :

$$Q_{\text{meas}} = Q_{\text{ref}} \times \frac{P_{\text{ref}}}{P_{\text{meas}}} \times \frac{T_{\text{meas}}}{T_{\text{ref}}}$$

where Q = Flow Rate P = Absolute Pressure T = Absolute Temperature

Meas = Measurement Condition ref = Standard Condition

**Note**

\* Indicates non accredited

\*\* Reference Specifications ± 5% of set flow or ± 3 cc/min whichever is higher

\*\*\* Specified in ISO 13137, Back Pressure control ± 1 inH<sub>2</sub>O

**End of Certificate**

**เอกสารไม่ควบคุม**



Certificate of Calibration

**Customer**  
Name : UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.  
Address : 81 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Prakanong, Bangkok  
10260

**Certificate No :** 24-ASP-122  
**Request No :** Req-2024-1795

Unit Under Calibration Details

Measurement Item : Air Sampling Pump  
Manufacturer : SENSIDYNE  
Model : GilAir Plus  
Serial Number : 20230610198  
ID : UAE.EFM.128/2566  
Location of Calibration : LAB 4 AIR VELOCITY METER  
Instrument Status : Used

Calibration Environment and Details

Temperature : 23 °C ± 3 °C  
Humidity : 55 %RH ± 20 %RH  
Barometric Pressure : 1013 hPa ± 10 hPa  
Received Date : 15 August 2024  
Calibration Date : 26 August 2024  
Calibration Procedure : In-house method CP-ASP-01 based on ISO 13137 by Comparison With Standard Air Flow Meter

Reference Standard	Model	Serial Number	Traceble	Due Calibration
Air Flow Meter	Gilibrator 3 Standard flow	19031011003	Sensidyne	2 August 2025
Digital Thermometer with Probe	GT11	08000057	Q.Reborn	1 March 2025
Barometer	CPG2400	41000KDU/651882	TPA	9 November 2024

**Traceability :**  
This Certificate is traceable to SI Unit through Sensidyne A2LA Accreditation No. 3943.01

**Note :**  
The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor  $k = 2$ , providing a level of confidence approximately 95 %.

**Calibration By :** me  
Mr. Noppadon Luangart  
Service Calibration Engineer

**Approved By :** Mr. Pacit Mathavorn  
Mr. Pacit Mathavorn  
Calibration Engineer Supervisor  
**Issue Date :** 26 August 2024

เอกสารไม่ควบคุม

Certificate No : 24-ASP-122

Request No : Req-2024-1795

Result of Calibration : Low (Without Adjustment)

Temperature (°C)	Pressure (kPa)	STD (l/min)	UUC (l/min)	Error (l/min)	Error (l/min), (%)	MPE (l/min), (%)	**Back Pressure (inH <sub>2</sub> O)	Uncertainty (l/min)	Result
24.10	99.37	0.021	0.020	-0.001	-0.001 l/min	0.003 l/min	5	0.0012	Pass
24.10	96.22	0.021	0.020	-0.001	-0.001 l/min	0.003 l/min	20	0.0012	Pass
24.10	91.82	0.021	0.020	-0.001	-0.001 l/min	0.003 l/min	40	0.0012	Pass
24.10	99.43	0.048	0.050	0.002	0.002 l/min	0.003 l/min	5	0.0026	Pass
24.10	95.57	0.050	0.050	0.000	0 l/min	0.003 l/min	20	0.0028	Pass
24.10	90.65	0.047	0.050	0.003	0.003 l/min	0.003 l/min	40	0.0026	Pass
24.10	99.49	0.099	0.100	0.001	1 (%)	5 (%)	5	0.0026	Pass
24.10	95.57	0.098	0.100	0.002	2 (%)	5 (%)	20	0.0025	Pass
24.10	90.78	0.100	0.100	0.000	0 (%)	5 (%)	40	0.0026	Pass
24.20	99.48	0.201	0.200	-0.001	-0.5 (%)	5 (%)	5	0.0036	Pass
24.20	96.03	0.201	0.200	-0.001	-0.5 (%)	5 (%)	20	0.0036	Pass
24.20	90.90	0.199	0.200	0.001	0.5 (%)	5 (%)	40	0.0036	Pass

เอกสารไม่ควบคุม



Certificate No : 24-ASP-122

Request No : Req-2024-1795

**Result of Calibration : High (Without Adjustment)**

Temperature (°C)	Pressure (kPa)	STD (l/min)	UUC (l/min)	Error (l/min)	Error (l/min), (%)	MPE (l/min), (%)	**Back Pressure (inH <sub>2</sub> O)	Uncertainty (l/min)	Result
24.00	99.47	0.500	0.500	0.000	0 %	5 (%)	5	0.0080	Pass
24.00	95.66	0.502	0.500	-0.002	-0.4 %	5 (%)	20	0.0080	Pass
24.00	91.97	0.498	0.500	0.002	0.4 %	5 (%)	40	0.0080	Pass
23.90	99.50	1.006	1.000	-0.006	-0.6 (%)	5 (%)	5	0.016	Pass
23.90	95.58	1.002	1.000	-0.002	-0.2 (%)	5 (%)	20	0.016	Pass
23.90	91.88	0.992	1.000	0.008	0.8 (%)	5 (%)	35	0.016	Pass
23.90	99.43	1.705	1.700	-0.005	-0.3 (%)	5 (%)	5	0.027	Pass
23.90	95.71	1.672	1.700	0.028	1.7 (%)	5 (%)	20	0.027	Pass
23.90	93.09	1.661	1.700	0.039	2.3 (%)	5 (%)	30	0.027	Pass
23.90	99.43	2.004	2.000	-0.004	-0.2 (%)	5 (%)	5	0.032	Pass
23.90	95.72	1.985	2.000	0.015	0.8 (%)	5 (%)	20	0.032	Pass
23.90	93.13	1.972	2.000	0.028	1.4 (%)	5 (%)	30	0.032	Pass
23.80	99.40	3.002	3.000	-0.002	-0.1 (%)	5 (%)	5	0.048	Pass
23.80	95.42	3.003	3.000	-0.003	-0.1 (%)	5 (%)	20	0.048	Pass
23.80	93.24	2.994	3.000	0.006	0.2 (%)	5 (%)	30	0.048	Pass
23.80	99.41	4.003	4.000	-0.003	-0.1 (%)	5 (%)	5	0.064	Pass
23.90	98.12	4.005	4.000	-0.005	-0.1 (%)	5 (%)	10	0.064	Pass
23.90	95.33	3.995	4.000	0.005	0.1 %	5 (%)	20	0.064	Pass
23.70	99.41	5.005	5.000	-0.005	-0.1 %	5 (%)	5	0.080	Pass
23.70	97.65	5.001	5.000	-0.001	0 %	5 (%)	12	0.080	Pass

**Note**

STD : Standard UUC : Unit Under Calibration

- UUC Reference Condition : At 25 °C, 101.3 kPa, Air

- Flow Rate was corrected for non-standard operating condition by using equation :

$$Q_{\text{meas}} = Q_{\text{ref}} \times \frac{P_{\text{ref}}}{P_{\text{meas}}} \times \frac{T_{\text{meas}}}{T_{\text{ref}}}$$

where Q = Flow Rate P = Absolute Pressure T = Absolute Temperature  
 meas = Measurement Condition ref = Standard Condition

**เอกสารไม่ควบคุม**

Certificate No : 24-ASP-122

Request No : Req-2024-1795

**Note**

\* Indicates non accredited

\*\* Specified in ISO 13137, Back Pressure control  $\pm 1$  inH2O

MPE = Maximum Permissible Error (Specified in Manufacturer's Specification)

**Decision Rule for Statements of Conformity**


The standard decision rule employed for the statements of conformity to each calibration result will be applied using ILAC-G8:09/2019: Guidelines on the Reporting of Compliance with Specification as following Fig. and statements

Pass = The measurement result plus the expanded uncertainty with a 95% coverage probability were within the limit.

Pass<sup>1</sup> = The measurement result was within the limit. However, a portion of the expanded uncertainty of measurement at 95% exceeds the limit.

Fail<sup>1</sup> = The measurement result was out of the limit. However, a portion of the expanded uncertainty of measurement at 95% is within the limit.

Fail = The measurement result plus the expanded uncertainty with a 95% coverage probability were outside the limit.

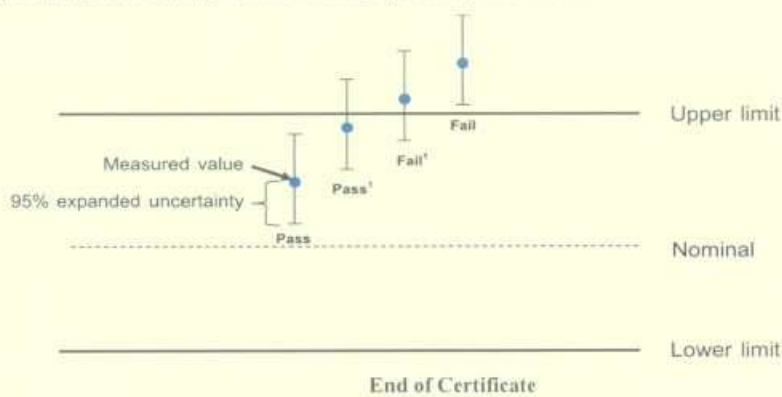

End of Certificate

**เอกสารไม่ควบคุม**



Certificate of Calibration

Customer

Name : UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.  
Address : 81 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Prakanong, Bangkok  
10260

Certificate No : 24-ASP-125

Request No : Req-2024-1792

Unit Under Calibration Details

Measurement Item : Air Sampling Pump  
Manufacturer : SENSIDYNE  
Model : GilAir Plus  
Serial Number : 20230610205  
ID : UAE.EFM.135/2566  
Location of Calibration : LAB 4 AIR VELOCITY METER

Instrument Status : Used

Calibration Environment and Details

Temperature : 23 °C ± 3 °C  
Humidity : 55 %RH ± 20 %RH  
Barometric Pressure : 1013 hPa ± 10 hPa  
Received Date : 15 August 2024  
Calibration Date : 27 August 2024  
Calibration Procedure : In-house method CP-ASP-01 based on ISO 13137 by Comparison With Standard Air Flow Meter

Reference Standard	Model	Serial Number	Traceble	Due Calibration
Air Flow Meter	Gilibrator 3 Standard flow	19031011003	Sensidyne	2 August 2025
Digital Thermometer with Probe	GT11	08000057	Q.Reborn	1 March 2025
Barometer	CPG2400	41000KDU/651882	TPA	9 November 2024

Traceability :

This Certificate is traceable to SI Unit through Sensidyne A2LA Accreditation No. 3943.01

Note :

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor  $k = 2$ , providing a level of confidence approximately 95 %.

Calibration By : Mr. Noppadon Luangart  
Service Calibration Engineer

Approved By : Mr. Pacit Mathavorn  
Calibration Engineer Supervisor

Issue Date : 27 August 2024

เอกสารไม่ควบคุม



Certificate No : 24-ASP-125

Request No : Req-2024-1792

Result of Calibration : Low (Without Adjustment)

Temperature (°C)	Pressure (kPa)	STD (l/min)	UUC (l/min)	Error (l/min)	Error (l/min), (%)	MPE (l/min), (%)	**Back Pressure (inH <sub>2</sub> O)	Uncertainty (l/min)	Result
25.20	98.77	0.021	0.020	-0.001	-0.001 l/min	0.003 l/min	5	0.0012	Pass
25.20	95.14	0.018	0.020	0.002	0.002 l/min	0.003 l/min	20	0.0010	Pass
25.20	90.64	0.017	0.020	0.003	0.003 l/min	0.003 l/min	40	0.0009	Pass
25.00	99.42	0.050	0.050	0.000	0 l/min	0.003 l/min	5	0.0028	Pass
25.00	96.05	0.051	0.050	-0.001	-0.001 l/min	0.003 l/min	20	0.0028	Pass
25.00	90.51	0.048	0.050	0.002	0.002 l/min	0.003 l/min	40	0.0026	Pass
24.90	99.55	0.099	0.100	0.001	1 (%)	5 (%)	5	0.0026	Pass
24.90	95.76	0.098	0.100	0.002	2 (%)	5 (%)	20	0.0025	Pass
24.90	90.91	0.097	0.100	0.003	3.1 (%)	5 (%)	40	0.0025	Pass
24.90	99.50	0.201	0.200	-0.001	-0.5 (%)	5 (%)	5	0.0036	Pass
24.90	95.69	0.199	0.200	0.001	0.5 (%)	5 (%)	20	0.0036	Pass
24.90	91.03	0.198	0.200	0.002	1 (%)	5 (%)	40	0.0036	Pass

**เอกสารไม่ควบคุม**

Certificate No : 24-ASP-125

Request No : Req-2024-1792

**Result of Calibration : High(Without Adjustment)**

Temperature (°C)	Pressure (kPa)	STD (l/min)	UUC (l/min)	Error (l/min)	Error (l/min), (%)	MPE (l/min), (%)	**Back Pressure (inH <sub>2</sub> O)	Uncertainty (l/min)	Result
24.80	99.47	0.503	0.500	-0.003	-0.6 %	5 (%)	5	0.0080	Pass
24.80	95.89	0.505	0.500	-0.005	-1 %	5 (%)	20	0.0081	Pass
24.80	91.72	0.499	0.500	0.001	0.2 %	5 (%)	40	0.0080	Pass
24.80	99.41	1.003	1.000	-0.003	-0.3 (%)	5 (%)	5	0.016	Pass
24.80	95.55	0.997	1.000	0.003	0.3 (%)	5 (%)	20	0.016	Pass
24.80	92.18	0.987	1.000	0.013	1.3 (%)	5 (%)	35	0.016	Pass
24.80	99.45	1.710	1.700	-0.010	-0.6 (%)	5 (%)	5	0.027	Pass
24.80	95.63	1.677	1.700	0.023	1.4 (%)	5 (%)	20	0.027	Pass
24.80	93.09	1.655	1.700	0.045	2.7 (%)	5 (%)	30	0.027	Pass
24.80	99.45	2.005	2.000	-0.005	-0.2 (%)	5 (%)	5	0.032	Pass
24.80	95.66	1.980	2.000	0.020	1 (%)	5 (%)	20	0.032	Pass
24.80	93.12	1.966	2.000	0.034	1.7 (%)	5 (%)	30	0.032	Pass
24.80	99.41	3.014	3.000	-0.014	-0.5 (%)	5 (%)	5	0.048	Pass
24.80	95.53	3.012	3.000	-0.012	-0.4 (%)	5 (%)	20	0.048	Pass
24.80	93.13	2.992	3.000	0.008	0.3 (%)	5 (%)	30	0.048	Pass
24.30	99.38	4.004	4.000	-0.004	-0.1 (%)	5 (%)	5	0.064	Pass
24.30	98.11	4.012	4.000	-0.012	-0.3 (%)	5 (%)	10	0.064	Pass
24.30	95.60	4.007	4.000	-0.007	-0.2 %	5 (%)	20	0.064	Pass
24.20	99.36	5.005	5.000	-0.005	-0.1 %	5 (%)	5	0.080	Pass
24.20	97.52	5.011	5.000	-0.011	-0.2 %	5 (%)	12	0.080	Pass

**Note** STD : Standard UUC : Unit Under Calibration

- UUC Reference Condition : At 25 °C, 101.3 kPa, Air

- Flow Rate was corrected for non-standard operating condition by using equation :

$$Q_{\text{meas}} = Q_{\text{ref}} \times \frac{P_{\text{ref}}}{P_{\text{meas}}} \times \frac{T_{\text{meas}}}{T_{\text{ref}}}$$

where Q = Flow Rate P = Absolute Pressure T = Absolute Temperature  
 meas = Measurement Condition ref = Standard Condition

**เอกสารไม่ควบคุม**



Certificate No : 24-ASP-125

Request No : Req-2024-1792

**Note**

\* Indicates non accredited

\*\* Specified in ISO 13137, Back Pressure control  $\pm 1$  inH2O

MPE = Maximum Permissible Error (Specified in Manufacturer's Specification)

**Decision Rule for Statements of Conformity**


The standard decision rule employed for the statements of conformity to each calibration result will be applied using ILAC-G8:09/2019: Guidelines on the Reporting of Compliance with Specification as following Fig. and statements

Pass = The measurement result plus the expanded uncertainty with a 95% coverage probability were within the limit.

Pass<sup>1</sup> = The measurement result was within the limit. However, a portion of the expanded uncertainty of measurement at 95% exceeds the limit.

Fail<sup>1</sup> = The measurement result was out of the limit. However, a portion of the expanded uncertainty of measurement at 95% is within the limit.

Fail = The measurement result plus the expanded uncertainty with a 95% coverage probability were outside the limit.

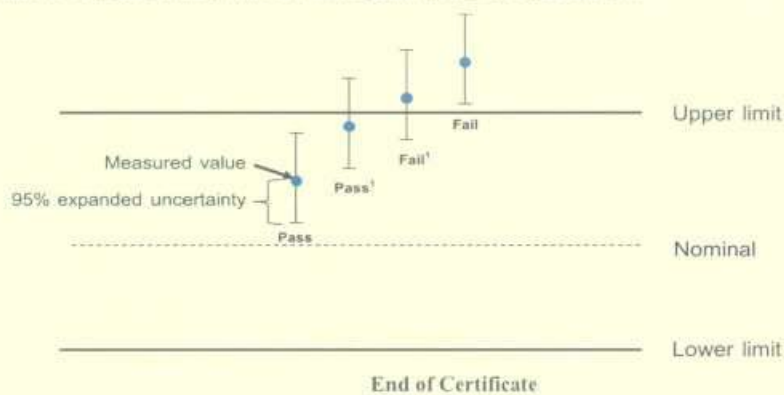

**เอกสารไม่ควบคุม**



## Certificate of Calibration

Certificate No. : 24P1370

Page : 1 of 2

**Equipment :** Aneroid Barometer  
**Manufacturer:** Barigo  
**Model :** 111MS  
**Serial No.:** -  
**ID No.:** UAE.EMA2.065/2552

**Condition As-Received:** Used Item

**Received Date:** 05 April 2024

**Calibration Date:** 22 April 2024

**Reference:** 2404-0243WSC

**Ambient Temperature:** ( 23 ± 2 ) °C

**Relative Humidity:** ( 50 ± 15 ) %

**Atmospheric Pressure:** 1007 mbar

**Submitted by:** United Analyst and Engineering Consultant Co.,Ltd.

81 Soi Udomsuk 41, Sukhumvit Road, Bangchak,  
Phrakhanong, Bangkok 10260

**Procedure used:** The calibration was conducted by direct comparison method against Pressure Measuring Instruments Standard according to calibration procedure CP-P10, using " DKD-R 6-1 ; Calibration of Pressure Gauges " as a guidelines.

### Condition of this result of calibration

1.Reference standards instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Certificate No.</u>	<u>Due Date</u>
1) Standard Barometer	DPI142	1422505046	MP-0094-23	03 May 2024

2.This instrument was installed in vertical orientation and center of the dial was used as the reference level.

3.This result of calibration was made on requested at the point specified by customer.

4.Scale and conversion factor is 1 kPa = 7.50062 mmHg

5.This result of calibration instrument was in absolute pressure.

6.This instrument was used clean air as pressure media.

7.The certificate is valid only to the item calibrated on date and place of calibration.

8.This Certification is traceable to the International System of Unit maintained through:-

-National Institute of Metrology Thailand (NIMT)

**Calibrated by :** Suksan Khankaew  
**Issue Date :** 23 April 2024

**Approved Signatory :** \_\_\_\_\_  
[ ] Phalinee Prabpaipal  
[ ] Sura Suwannasri  
[✓] Attapol Panurach

เอกสารไม่ควบคุม



Cert.No.: 24P1370

Page: 2 of 2

**Result of calibration:- Without adjustment**

**Range :** 720 mmHg to 770 mmHg

**Function:- Absolute Pressure Measurement**

**Scale Interval :** 1 mmHg ( The Fifth Estimate )

**Increasing Pressure**

Applied Pressure (mmHg)	715.75	726.88	738.53	749.84	761.99	774.19
UUC* Indication (mmHg)	720.0	730.0	740.0	750.0	760.0	770.0
Error (mmHg)	4.25	3.12	1.47	0.16	-1.99	-4.19

**Decreasing Pressure**

Applied Pressure (mmHg)	774.19	761.85	749.40	738.00	726.53	715.75
UUC* Indication (mmHg)	770.0	760.0	750.0	740.0	730.0	720.0
Error (mmHg)	-4.19	-1.85	0.60	2.00	3.47	4.25

The uncertainty of measurement was  $\pm 0.24$  mmHg

\* UUC = Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor  $k = 2$ , providing a level of confidence of approximately 95 %.

-oOo-

เอกสารไม่ควบคุม





TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)  
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES  
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG, BANGKOK 10250  
TEL. 0-2717-3000-24 FAX. 0-2719-9484



## Certificate of Calibration

Certificate No. : 24H717

Page : 1 of 2

Equipment : Digital Thermo-Hygrometer  
Manufacturer: Digicon  
Model : TH-02  
Serial No.: 395034172  
ID No.: UAE.EFM.181/2565

This certificate may not be reproduced other than in full,  
except with the prior written approval of the head of  
Corporate Services 3: Equipment Calibration and Testing Services.

Condition As-Received: Used Item

Received Date: 05 April 2024

Calibration Date: 10 April 2024  
to 11 April 2024

Reference: 2404-0245WSC

Submitted by: United Analyst and Engineering Consultant Co.,Ltd.

Ambient Temperature: ( 25 ± 3 ) °C

Relative Humidity: ( 50 ± 20 ) %

81 Soi Udomsuk 41, Sukhumvit Road,  
Bangchak, Phrakhanong, Bangkok 10260

Procedure used: Calibration were conducted using in-house calibration procedure CP-H03 according to comparison with standard chilled mirror sensor for humidity measurement function and comparison with standard temperature probe for temperature measurement function into humidity / temperature chamber.

### Condition of this result of calibration

1.Reference standards instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Certificate No.</u>	<u>Due Date</u>
1) Chilled Mirror Hygrometer	Dew Master	44730	21656	02 Aug 2024
2) Handheld Thermometer With Sensor	1521	A5A339	2311238	16 Oct 2024

2.The certificate is valid only to the item calibrated on date and place of calibration.

3.This Certification is traceable to the International System of Unit maintained through:-

- Thunder Scientific Corporation, NVLAB Accreditation No. Calibration 200582-0
- Technology Promotion Association (Thailand-Japan), NSC-ONSC Accredited No. Calibration 0008

Calibrated by : Viporn Tantiyawutti  
Issue Date : 17 April 2024

Approved Signatory :

- ☒ Chakrit Waewwanjua  
☐ Viporn Tantiyawutti  
☐ Unnopphol Harachai

เอกสารไม่ควบคุม

B 0339074



Cert. No.: 24H717

Page.: 2 of 2

**Result of Calibration:-** Without Adjustment

**Function:** Humidity Measurement.

<u>Reference</u> <u>Temperature</u> (°C)	<u>Standard</u> <u>Humidity</u> (%R.H.)	<u>UUC*</u> <u>Reading</u> (%R.H.)	<u>Error</u> (%R.H.)	<u>Uncertainty</u> <u>of Measurement</u> (±%R.H.)
25.0	40.1	42	1.9	1.3
25.0	50.1	52	1.9	1.6
25.0	60.0	60	0.0	1.6
25.0	70.2	68	-2.2	1.6

**Result of Calibration:-** Without Adjustment

**Function:** Temperature Measurement.

<u>Standard</u> <u>Temperature</u> (°C)	<u>UUC*</u> <u>Reading</u> (°C)	<u>Error</u> (°C)	<u>Uncertainty</u> <u>of Measurement</u> (±°C)
19.998	20.2	0.202	0.42
25.031	25.4	0.369	0.42
30.045	30.1	0.055	0.42
40.023	39.9	-0.123	0.42

**UUC\*** : Unit Under Calibration

The reported uncertainty of measurement was base on standard uncertainty multiplied by coverage factor  $k = 2.00$ , providing confidence level approximately 95%.

-o0o-

เอกสารไม่ควบคุม

a 1210372





# บริษัท เอกเสคคิวทิฟเทรดดิ้ง จำกัด (สำนักงานใหญ่)

48/194-5 ซอยประดิษฐ์มนูธรรม 19 ถนนประดิษฐ์มนูธรรม แขวงลาดพร้าว เขตลาดพร้าว กรุงเทพฯ 10230  
TEL (662) 515-0145-50 FAX (662) 515-0144 www.etlthai.com E-mail : info@etlthai.com

No. RA 187/24

## Certificate of Calibration

**Customer** : United Analyst and Engineering Consultant Co., Ltd.  
**Address** : 81 Soi Udomsuk 41, Sukhumvit Road., Bangchak, Prakanong, Bangkok, 10260.  
**Calibration location** : Executive Trading Limited.  
**Address** : 48/194-5 Soi Praditmanutham 19, Pradit Manutham Road, Latphrao, Bangkok 10230

### Tools :

**Instrument** : Gas Detector  
**Product** : RAE Systems  
**Model Name** : MiniRAE3000+  
**Serial Number** : 592-928075

### Environmental Condition :

**Temperature** :  $(25 \pm 3) ^\circ\text{C}$   
**Relative Humidity** :  $(39 \pm 15) \%$   
**Pressure** : 760 mmHg

Tag ID. : UAE.EFM.124/2562.

**Date of Calibration** : August 7, 2024

**Due Date of Calibration** : August 7, 2025

**Calibration Method** : This instrument has been calibrated using calibration gases. Test and calibration data is  
On file with Executive trading limited.

**Reference Standard** : Isobutylene Standard Gas 100 Cylinder number: WO349099-1.  
Exp Date: 25 April 2027.

### Test Result

Sensor Type	Reference Concentration	Before Cal.	After Cal.	Error Reading	Result
PID	0.0 ppm (Air Zero)	0.0 ppm	0.0 ppm	0.0 ppm	Pass
PID	100 ppm (Isobutylene)	102.3 ppm	100.0 ppm	0.0 ppm	Pass

**Flow Rate of Pump** : 484 cc/min.

**Accuracy** :  $\pm 2 \%$  at calibration point

Calibrated By : Surinthorn S.

(Mr. Surinthorn Sainate)

Service Engineer

Approved By : Suttiwong

(Mr. Suttiwong Kongtongsang.)

Service Engineer Manager

The results relate only to the items tested or calibrated.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the company.

เอกสารไม่ควบคุม

## Certificate of Calibration

### Customer

Name : UNITED ANALYST AND ENGINEERING  
CONSULTANT CO.,LTD.  
Address : 81 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Prakanong,  
Bangkok 10260

Certificate No : 24-ACT-067  
Request No : Req-2024-1024

### Unit Under Calibration Details

Measurement item : Acoustic Calibrator Class : 2  
Manufacturer : LARSON DAVIS Range : 94 , 114 dB / 1000 Hz  
Model : CAL150 Instrument Status : Used  
Serial Number : 6306  
ID : UAE.EFM.048/2563

### Calibration Environment and Details


Temperature : ( 23 ±2 °C )  
Humidity : ( 50 ± 20 %RH )  
Barometric Pressure : ( 1013 ±10.0 hPa )  
Received Date : 8 May 2024  
Calibration Date : 17 May 2024  
Location of Calibration : LAB 1 Acoustic  
Calibration Procedure : In-house method CP-ACT-02 based on IEC 60942:2017 Electroacoustics - Sound calibrators


Reference Standard	Model	Serial Number	Traceable	Due Calibration
Sound Calibrator	SV 35A	58079	EEI	31 May 2024
THD Multimeter	2015	1047765	NIMT	16 January 2025

**Traceability** : This certificate provides traceability of measurement to recognized national standard, and to the realization of the international System of Units (SI).

### Note

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor k=2, providing a level of confidence approximately 95 %.

Calibrated By :   
Mr. Noppadon Luangart  
Service Calibration Engineer

Approved By :   
Mr. Pacit Mathavorn  
Calibration Engineer Supervisor

Issue Date : 17 May 2024

Certificate No : 24-ACT-067

Request No : Req-2024-1024

**Sound pressure level**

**Calibration Results : Without Adjustment**

Calibration Range (dB)	Without Adjustment (dB)		Adjustment (dB)		Uncertainty ( ± dB)	Acceptance limit Class 2 ( ± dB)
	Measured	Deviated value	Measured	Deviated value		
94 dB / 1000 Hz	94.09	0.09	-	-	0.13	0.40
114 dB / 1000 Hz	114.10	0.10	-	-	0.13	0.40

**Frequency of Sound pressure level**

Calibration Range (Hz)	Without Adjustment		Adjustment		Uncertainty ( ± %)	Acceptance limit Class 2 ( ± %)
	Measured (Hz)	Deviated value	Measured (Hz)	Deviated value		
94 dB / 1000 Hz	1000.00	0.00	-	-	0.01	1.7
114 dB / 1000 Hz	1000.00	0.00	-	-	0.01	1.7

**Total Harmonic Distortion plus Noise of Sound pressure level (THD+N %)**

Calibration Range (Hz)	Without Adjustment	Adjustment	Uncertainty ( ± %)	Acceptance limit Class 2 ( ± %)
	Measured (%)	Measured (%)		
94 dB / 1000 Hz	0.05	-	0.40	3.0
114 dB / 1000 Hz	0.21	-	0.40	3.0

**Note :**

Function	Maximum-permitted Uncertainty of measurement
Sound pressure level	0.35 dB
Frequency	0.20%
Total distortion+noise	1.00%

- Acceptance limit was IEC60942:2017 Class 1

- The calibration results exclude the calibrator pressure correction

- The calibration results exclude the microphone volume correction

**End of Calibration**



Cert. No. : ACL24061

Pages : 1 of 8

## Calibration Certificate

**Equipment :** SOUND LEVEL METER  
**Manufacturer :** RION  
**Model :** NL-42 / Microphone UC-52 / Preamplifier NH-24  
**Serial No.:** 00709670 / 188531 / 01221  
**ID No.:** UAE.EFM.022/2564

**Condition As Found :** GOOD

**Customer :** UNITED ANALYST AND ENGINEERING CONSULTANT (UAE)  
81 SOI UDOMSUK 41, SUKHUMVIT ROAD,  
BANGCHAK SUB-DISTRICT,  
PHRAKHANONG DISTRICT, BANGKOK 10260  
THAILAND.

**Location :** -

**Ambient Temperature :** ( 23.0  $\pm$  3 ) °C  
**Pressure :** ( 101.3  $\pm$  3 ) kPa  
**Relative Humidity :** ( 50.0  $\pm$  20 ) %

**Received Date :** 21 DECEMBER 2023  
**Calibration Date :** 18-19 JANUARY 2024  
**Date of Issue :** 22 JANUARY 2024

**Calibrated by :**

Nathakorn Pisutpaisan

**Approved by :**

  
( Thanakul Petchurai )

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

เอกสารไม่ควบคุม

# SITHIPORN ASSOCIATES CO., LTD.

## CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand  
Tel, +66 2433 8331 Email : calibration@sithiporn.com



Cert. No. : ACL24061  
Job No. : VC67AC0034  
Pages : 2 of 8

**Calibration Procedure :** CP-AC-01

### Calibration Method :

This equipment was calibrated by follow on IEC-61672-3 (2013) Standard for sound level meter (SLM).

The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.

For tests results of each items were made by observation of each Instruments display and also with SLM's display.

### Condition of this result of calibration :

#### 1. Reference Standard Instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
Waveform Generator	33210A	MY48017076	EF-0009-23	07-FEB-24
Waveform Generator	33511B	MY52302742	EF-0010-23	07-FEB-24
Digital Multimeter	33461A	MY53220104	EEL.BP 30/0266	13-FEB-24
Digital Multimeter	33461A	MY53220076	EEL.BP 29/0266	13-FEB-24
Digital Multimeter	34461A	MY60024273	EEL.BP 31/0266	14-FEB-24
Programmable Attenuator	MAT-1070	62100114	EF-0011-23	08-FEB-24
Condenser Microphone	4180	2977900	AA-1001-23	14-FEB-24
Measuring Amplifier	NA-42KAI	34560495	AA-3002-23	14-FEB-24

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is traceable to the international system of unit maintained at :

3.1 National Institute of Metrology (Thailand).

3.2 Thailand Institute of Scientific and Technological Research (TISTR).

เอกสารไม่ควบคุม  
*[Signature]*



# SITHIPORN ASSOCIATES CO., LTD.

## CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand  
Tel. +66 2433 8331 Email : calibration@sithiporn.com

SITHIPORN  
associates



Cert. No. : ACL24061  
Job No. : VC67AC0034  
Pages : 3 of 8

### Summary of Measurement Result :

Parameter	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	0.2	N/A
2. Self-generated noise	0.2	N/A
3. Acoustical signal tests of frequency weightings		
125 Hz	0.3	0.6
1000 Hz	0.3	0.6
8000 Hz	0.3	0.7
4. Electrical signal tests of frequency weightings		
For 10 Hz to 4 kHz	0.3	0.6
For > 4 kHz to 10 kHz	0.3	0.7
For > 10 kHz to 20 kHz	-	1.0
5. Frequency and time weightings at 1 kHz	0.2	0.2
6. Long - term stability	0.1	0.1
7. Level linearity on the reference level range	0.2	0.3
8. Level linearity including the level range control	0.2	0.3
9. Tone burst response	0.2	0.3
10. Peak C sound level	0.2	0.35
11. Overload indication	0.2	0.25
12. High level stability	0.1	0.1

เอกสารไม่ควบคุม  
7. Kewh

# SITHIPORN ASSOCIATES CO., LTD.

## CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand  
Tel. +66 2433 8331 Email : calibration@sithiporn.com

SITHIPORN  
associates



Cert. No. : ACL24061

Job No. : VC67AC0034

Pages : 4 of 8

### Result of calibration :

#### 1. Absolute sensitivity

Reference Acoustic Signal ( dB )	Measured Value ( dB )	Deviation ( dB )	Acceptance Limit ( dB )
93.9 (93.98)	93.9	0.0	±0.3

#### 2. Self-generated noise

##### 2.1 Normal test

Measured Value ( dB )
15.4

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Measured value ( dB )
A - weight	12.0
C - weight	18.2
Flat	23.9

#### 3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency ( Hz )	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
125	0.0	0.0	0.0	± 1.5
1000	0.1	0.1	0.1	± 1.0
8000	3.0	3.1	3.1	±5.0

เอกสารไม่ควบคุม  
7. Kell...

**Cert. No. : ACL24061**  
**Job No. : VC67AC0034**  
**Pages : 5 of 8**

#### 4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency ( Hz )	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	0.0	-0.1	0.0	±2.0
125	0.0	0.1	0.0	±1.5
250	0.0	0.0	0.0	±1.5
500	0.0	0.1	0.0	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.1	0.0	±2.0
4000	0.0	0.0	0.0	±3.0
8000	0.0	0.1	0.1	±5.0

#### 5. Frequency and time weightings at 1 kHz

##### 5.1 Frequency weightings at 1 kHz

Frequency Weighting	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	94.0	94.0	0.0	± 0.2
C - weight	94.0	94.0	0.0	± 0.2
Flat	94.0	94.0	0.0	± 0.2

##### 5.2 Time weighting at 1 kHz

Frequency Weighting	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Fast	94.0	94.0	0.0	± 0.1
Slow	94.0	94.0	0.0	± 0.1
Leq	94.0	94.0	0.0	± 0.1

#### 6. Long - term stability

Frequency Weighting	SLM Display at initial ( dB )	SLM Display at final ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	94.0	94.1	0.1	± 0.3

เอกสารไม่ควบคุม

*F. Kewin*

# SITHIPORN ASSOCIATES CO., LTD.

## CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand  
Tel. +66 2433 8331 Email : calibration@sithiporn.com

SITHIPORN  
associates



Cert. No. : ACL24061

Job No. : VC67AC0034

Pages : 6 of 8

### 7. Level linearity on the reference level range

Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
137.0	137.0	0.0	$\pm 1.1$
136.0	136.0	0.0	$\pm 1.1$
135.0	135.0	0.0	$\pm 1.1$
134.0	134.0	0.0	$\pm 1.1$
133.0	133.0	0.0	$\pm 1.1$
132.0	132.0	0.0	$\pm 1.1$
131.0	131.0	0.0	$\pm 1.1$
129.0	129.0	0.0	$\pm 1.1$
124.0	124.0	0.0	$\pm 1.1$
119.0	119.0	0.0	$\pm 1.1$
114.0	114.0	0.0	$\pm 1.1$
109.0	109.0	0.0	$\pm 1.1$
104.0	104.0	0.0	$\pm 1.1$
99.0	99.0	0.0	$\pm 1.1$
94.0	94.0	0.0	$\pm 1.1$
89.0	89.0	0.0	$\pm 1.1$
84.0	84.0	0.0	$\pm 1.1$
79.0	79.0	0.0	$\pm 1.1$
74.0	74.0	0.0	$\pm 1.1$
69.0	69.0	0.0	$\pm 1.1$
64.0	64.0	0.0	$\pm 1.1$
59.0	59.0	0.0	$\pm 1.1$
54.0	54.0	0.0	$\pm 1.1$
49.0	49.0	0.0	$\pm 1.1$
44.0	44.0	0.0	$\pm 1.1$
39.0	39.0	0.0	$\pm 1.1$
34.0	34.0	0.0	$\pm 1.1$
30.0	30.0	0.0	$\pm 1.1$
29.0	28.9	-0.1	$\pm 1.1$
28.0	28.0	0.0	$\pm 1.1$
27.0	26.9	-0.1	$\pm 1.1$
26.0	25.9	-0.1	$\pm 1.1$
25.0	24.9	-0.1	$\pm 1.1$

เอกสารไม่ควบคุม  
T. Kewin



**Cert. No. : ACL24061**  
**Job No. : VC67AC0034**  
**Pages : 7 of 8**

**8. Level linearity including the level range control**

Range	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Auto	94.0	94.0	0.0	±1.1

**9. Tone burst response**

Time Weighting	Tone burst duration, Tb ( ms )	Cycle	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Fast	0.25	1	108.0	108.0	0.0	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.1	0.1	±1.0
Slow	2	8	108.0	108.0	0.0	1.5 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
SEL	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.0	0.0	±1.0

**10. Peak C sound level**

Number of cycle in test signal	Anticipated Value ( dB )	Measured Value, Lcpeak ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Continuous	133.0	133.0	0.0	±3.0
One	136.4	135.4	-1.0	±3.0

Number of cycle in test signal	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Continuous	133.0	133.1	0.1	±2.0
Positive half cycle	135.4	135.2	-0.2	±2.0
Negative half cycle	135.4	135.2	-0.2	±2.0

**เอกสารไม่ควบคุม**  
*G. Kelun*



# SITHIPORN ASSOCIATES CO., LTD.

## CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbunru, Bangplud, Bangkok, 10700 Thailand  
Tel. +66 2433 8331 Email : calibration@sithiporn.com

SITHIPORN  
associates



Cert. No. : ACL24061  
Job No. : VC67AC0034  
Pages : 8 of 8

### 11. Overload indication

Measured value ( dB )		Deviated Value ( dB )	Acceptance Limits ( dB )
Positive one-half cycle	Negative one-half cycle		
89.5	89.5	0.0	±1.5

### 12. High level stability

Frequency Weighting	SLM Display at initial ( dB )	SLM Display at final ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	137.0	137.1	-0.1	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor  $k = 2$   
or any value following calculation, providing a level of confidence of approximately 95 %

————— End of Calibration Certificate —————

เอกสารไม่ควบคุม  
*T. Keler*

Cert. No. : ACL24058

Pages : 1 of 8

## Calibration Certificate

**Equipment :** SOUND LEVEL METER  
**Manufacturer :** RION  
**Model :** NL-42 / Microphone UC-52 / Preamplifier NH-24  
**Serial No.:** 00609500 / 189689 / 01126  
**ID No.:** UAE.EFM.018/2564

**Condition As Found :** GOOD

**Customer :** UNITED ANALYST AND ENGINEERING CONSULTANT (UAE)  
81 SOI UDOMSUK 41, SUKHUMVIT ROAD,  
BANGCHAK SUB-DISTRICT,  
PHRAKHANONG DISTRICT, BANGKOK 10260  
THAILAND.

**Location :** -

**Ambient Temperature :** ( 23.0  $\pm$  3 ) °C  
**Pressure :** ( 101.3  $\pm$  3 ) kPa  
**Relative Humidity :** ( 50.0  $\pm$  20 ) %

**Received Date :** 21 DECEMBER 2023  
**Calibration Date :** 18-19 JANUARY 2024  
**Date of Issue :** 22 JANUARY 2024

**Calibrated by :**

Nathakorn Pisutpaisan

**Approved by :**

  
( Thanakul Petchurai )

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

เอกสารไม่ควบคุม

# SITHIPORN ASSOCIATES CO., LTD.

## CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbunru, Bangplud, Bangkok, 10700 Thailand  
Tel. +66 2433 8331 Email : calibration@sithiporn.com



Cert. No. : ACL24058  
Job No. : VC67AC0034  
Pages : 2 of 8

Calibration Procedure : CP-AC-01

### Calibration Method :

This equipment was calibrated by follow on IEC-61672-3 (2013) Standard for sound level meter (SLM).

The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.

For tests results of each items were made by observation of each Instruments display and also with SLM's display.

### Condition of this result of calibration :

#### 1. Reference Standard Instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
Waveform Generator	33210A	MY48017076	EF-0009-23	07-FEB-24
Waveform Generator	33511B	MY52302742	EF-0010-23	07-FEB-24
Digital Multimeter	33461A	MY53220104	EEL.BP 30/0266	13-FEB-24
Digital Multimeter	33461A	MY53220076	EEL.BP 29/0266	13-FEB-24
Digital Multimeter	34461A	MY60024273	EEL.BP 31/0266	14-FEB-24
Programmable Attenuator	MAT-1070	62100114	EF-0011-23	08-FEB-24
Condenser Microphone	4180	2977900	AA-1001-23	14-FEB-24
Measuring Amplifier	NA-42KAI	34560495	AA-3002-23	14-FEB-24

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is traceable to the international system of unit maintained at :

3.1 National Institute of Metrology (Thailand).

3.2 Thailand Institute of Scientific and Technological Research (TISTR).

เอกสารไม่ควบคุม  
9. Kew

# SITHIPORN ASSOCIATES CO., LTD.

## CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand  
Tel. +66 2433 8331 Email : calibration@sithiporn.com

SITHIPORN  
associates



Cert. No. : ACL24058

Job No. : VC67AC0034

Pages : 3 of 8

### Summary of Measurement Result :

Parameter	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	0.2	N/A
2. Self-generated noise	0.2	N/A
3. Acoustical signal tests of frequency weightings		
125 Hz	0.3	0.6
1000 Hz	0.3	0.6
8000 Hz	0.3	0.7
4. Electrical signal tests of frequency weightings		
For 10 Hz to 4 kHz	0.3	0.6
For > 4 kHz to 10 kHz	0.3	0.7
For > 10 kHz to 20 kHz	-	1.0
5. Frequency and time weightings at 1 kHz	0.2	0.2
6. Long - term stability	0.1	0.1
7. Level linearity on the reference level range	0.2	0.3
8. Level linearity including the level range control	0.2	0.3
9. Tone burst response	0.2	0.3
10. Peak C sound level	0.2	0.35
11. Overload indication	0.2	0.25
12. High level stability	0.1	0.1

เอกสารไม่ควบคุม  
*G. Kewin*



# SITHIPORN ASSOCIATES CO., LTD.

## CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand  
Tel. +66 2433 8331 Email : calibration@sithiporn.com

SITHIPORN  
associates



Cert. No. : ACL24058

Job No. : VC67AC0034

Pages : 4 of 8

### Result of calibration :

#### 1. Absolute sensitivity

Reference Acoustic Signal ( dB )	Measured Value ( dB )	Deviation ( dB )	Acceptance Limit ( dB )
93.9 (93.98)	93.9	0.0	±0.3

#### 2. Self-generated noise

##### 2.1 Normal test

Measured Value ( dB )
18.2

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Measured value ( dB )
A - weight	14.4
C - weight	20.7
Flat	26.5

#### 3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency ( Hz )	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
125	0.0	0.0	0.0	± 1.5
1000	-0.1	-0.1	-0.1	± 1.0
8000	1.4	1.5	1.5	±5.0

เอกสารไม่ควบคุม  
7. Kellin



**Cert. No. : ACL24058**  
**Job No. : VC67AC0034**  
**Pages : 5 of 8**

#### 4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency ( Hz )	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	0.0	0.0	0.0	±2.0
125	0.1	0.1	0.0	±1.5
250	0.0	0.0	0.0	±1.5
500	0.0	0.1	0.0	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.1	0.0	±2.0
4000	0.0	0.0	0.0	±3.0
8000	0.0	0.1	0.1	±5.0

#### 5. Frequency and time weightings at 1 kHz

##### 5.1 Frequency weightings at 1 kHz

Frequency Weighting	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	94.0	94.0	0.0	± 0.2
C - weight	94.0	94.0	0.0	± 0.2
Flat	94.0	94.0	0.0	± 0.2

##### 5.2 Time weighting at 1 kHz

Frequency Weighting	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Fast	94.0	94.0	0.0	± 0.1
Slow	94.0	94.0	0.0	± 0.1
Leq	94.0	94.0	0.0	± 0.1

#### 6. Long - term stability

Frequency Weighting	SLM Display at initial ( dB )	SLM Display at final ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	94.0	94.0	0.0	± 0.3

เอกสารไม่ควบคุม

7. Kewin

# SITHIPORN ASSOCIATES CO., LTD.

## CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand  
Tel. +66 2433 8331 Email : calibration@sithiporn.com

SITHIPORN  
associates



Cert. No. : ACL24058

Job No. : VC67AC0034

Pages : 6 of 8

### 7. Level linearity on the reference level range

Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
137.0	137.0	0.0	$\pm 1.1$
136.0	136.0	0.0	$\pm 1.1$
135.0	135.0	0.0	$\pm 1.1$
134.0	134.0	0.0	$\pm 1.1$
133.0	133.0	0.0	$\pm 1.1$
132.0	132.0	0.0	$\pm 1.1$
131.0	131.0	0.0	$\pm 1.1$
129.0	129.0	0.0	$\pm 1.1$
124.0	124.0	0.0	$\pm 1.1$
119.0	119.0	0.0	$\pm 1.1$
114.0	114.0	0.0	$\pm 1.1$
109.0	109.0	0.0	$\pm 1.1$
104.0	104.0	0.0	$\pm 1.1$
99.0	99.0	0.0	$\pm 1.1$
94.0	94.0	0.0	$\pm 1.1$
89.0	89.0	0.0	$\pm 1.1$
84.0	84.0	0.0	$\pm 1.1$
79.0	79.0	0.0	$\pm 1.1$
74.0	74.0	0.0	$\pm 1.1$
69.0	69.0	0.0	$\pm 1.1$
64.0	64.0	0.0	$\pm 1.1$
59.0	59.0	0.0	$\pm 1.1$
54.0	54.0	0.0	$\pm 1.1$
49.0	49.0	0.0	$\pm 1.1$
44.0	44.0	0.0	$\pm 1.1$
39.0	39.0	0.0	$\pm 1.1$
34.0	34.1	0.1	$\pm 1.1$
30.0	30.1	0.1	$\pm 1.1$
29.0	29.2	0.2	$\pm 1.1$
28.0	28.2	0.2	$\pm 1.1$
27.0	27.3	0.3	$\pm 1.1$
26.0	26.4	0.4	$\pm 1.1$
25.0	25.5	0.5	$\pm 1.1$

เอกสารไม่ควบคุม  
7. Kelvin.

# SITHIPORN ASSOCIATES CO., LTD.

## CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand  
Tel, +66 2433 8331 Email : calibration@sithiporn.com

SITHIPORN  
associates



Cert. No. : ACL24058  
Job No. : VC67AC0034  
Pages : 7 of 8

### 8. Level linearity including the level range control

Range	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Auto	94.0	94.0	0.0	±1.1

### 9. Tone burst response

Time Weighting	Tone burst duration, Tb ( ms )	Cycle	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.1	0.1	±1.0
Slow	2	8	108.0	108.0	0.0	1.5 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
SEL	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.1	0.1	±1.0

### 10. Peak C sound level

Number of cycle in test signal	Anticipated Value ( dB )	Measured Value, Lcpeak ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Continuous	133.0	133.0	0.0	±3.0
One	136.4	136.3	-0.1	±3.0

Number of cycle in test signal	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Continuous	133.0	133.0	0.0	±2.0
Positive half cycle	135.4	135.1	-0.3	±2.0
Negative half cycle	135.4	135.1	-0.3	±2.0

เอกสารไม่ควบคุม  
7. Kewin

# SITHIPORN ASSOCIATES CO., LTD. CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbunru, Bangplud, Bangkok, 10700 Thailand  
Tel. +66 2433 8331 Email : calibration@sithiporn.com

SITHIPORN  
associates



Cert. No. : ACL24058

Job No. : VC67AC0034

Pages : 8 of 8

## 11. Overload indication

Measured value ( dB )		Deviated Value ( dB )	Acceptance Limits ( dB )
Positive one-half cycle	Negative one-half cycle		
89.6	89.5	-0.1	±1.5

## 12. High level stability

Frequency Weighting	SLM Display at initial ( dB )	SLM Display at final ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor  $k = 2$   
or any value following calculation, providing a level of confidence of approximately 95 %

End of Calibration Certificate

เอกสารไม่ควบคุม  
7. Kelen





Certificate of Calibration

Customer

Name : UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.  
Address : 81 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Prakanong, Bangkok  
10260

Certificate No : 24-TPM-313  
Request No : Req-2024-1485  
Page : 1/2

Unit Under Calibration Details

Calibration Parameter	: Temperature	Range Calibration	: 20 °C to 60 °C
Instrument Name	: Thermal Environment Monitor	Type of Sensor	: RTD
Manufacturer	: TSI QUEST	Sensor Diameter (mm)	: 4.5
Model	: QT-34	Calibration Position (mm)	: 67.5
Serial Number	: TEX040015	Instrument Status	: Used
Resolution	: 0.1 °C		
ID Number	: UAE.EFM.119/2566		

Calibration Environment and Details

Temperature : 23 °C ± 3 °C  
Humidity : 55 %RH ± 15 %RH  
Received Date : 3 July 2024  
Calibrated Date : 9 July 2024  
Calibration Procedure : In-house method CP-TPM-01 by Comparison with Standard Thermometer.

Reference Standard : Digital Thermometer with Sensor, Manufacturer: GINGO/GINGO, Model: GT11/ RTD100, SN: 08000057, ID: 02-TPM  
Which was calibrated on 1 March 2024, Calibration Certificate No. : QR24-0478

Traceability : This Certificate is traceable to SI Unit through Quality Reborn Co., Ltd., NSC-ONSC Accreditation No.: Calibration 0292

Note

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor  $k=2$ , providing a level of confidence approximately 95 %.

Approved By :

me

Mr. Noppadon Luangart  
Technical Manager

Issue Date :

10 July 2024

เอกสารไม่ควบคุม



Calibration Note  
UUC Adjustment : Not Adjust  
Request No : Req-2024-1485  
Certificate No : 24-TPM-313

Page : 2/2

Result of Calibration :

UUC Sensor	Standard Temperature (°C)	UUC Reading (°C)	Correction (°C)	Uncertainty (± °C)
	20.032	20.0	0.0	0.13
WET	25.032	25.0	0.0	0.13
	30.031	30.1	- 0.1	0.13
	35.037	35.1	- 0.1	0.13
	40.040	40.2	- 0.2	0.13
	45.038	45.1	- 0.1	0.13
	50.042	50.2	- 0.2	0.13
	60.045	60.3	- 0.3	0.13

DRY	20.033	20.0	0.0	0.13
	25.030	25.0	0.0	0.13
	30.033	30.1	- 0.1	0.13
	35.034	35.1	- 0.1	0.13
	40.039	40.2	- 0.2	0.13
	45.038	45.1	- 0.1	0.13
	50.042	50.2	- 0.2	0.13
	60.046	60.3	- 0.3	0.13

GLOBE	20.033	19.9	+ 0.1	0.13
	25.030	25.1	- 0.1	0.13
	30.033	30.0	0.0	0.13
	35.035	35.0	0.0	0.13
	40.038	40.1	- 0.1	0.13
	45.041	45.1	- 0.1	0.13
	50.040	50.1	- 0.1	0.13
	60.045	60.1	- 0.1	0.13

End of Certificate

Calibrated By :

Mr. Sitichok Jirapukdeesakul

เอกสารแนบ

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

## Certificate of Calibration

### Customer

Name : UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.  
Address : 81 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Prakanong, Bangkok  
10260

Certificate No : 24-TPM-371

Request No : Req-2024-1693

Page : 1/2

### Unit Under Calibration Details

Calibration Parameter	: Temperature	Range Calibration	: 20 °C to 60 °C
Instrument Name	: Thermal Environment Monitor	Type of Sensor	: RTD
Manufacturer	: TSI QUEST	Sensor Diameter (mm)	: 4.5
Model	: QT-34	Calibration Position (mm)	: 67.5
Serial Number	: TEK120020	Instrument Status	: Used
Resolution	: 0.1 °C		
ID Number	: UAE.EMA2.023/2555		

### Calibration Environment and Details

Temperature : 23 °C ± 3 °C  
Humidity : 55 %RH ± 15 %RH  
Received Date : 2 August 2024  
Calibrated Date : 15 August 2024  
Calibration Procedure : In-house method CP-TPM-01 by Comparison with Standard Thermometer.

**Reference Standard** : Digital Thermometer with Sensor, Manufacturer: GINGO/GINGO, Model: GT11/ RTD100, SN: 08000057, ID: 02-TPM  
Which was calibrated on 1 March 2024, Calibration Certificate No. : QR24-0478

**Traceability** : This Certificate is traceable to SI Unit through Quality Reborn Co., Ltd., NSC-ONSC Accreditation No.: Calibration 0292

### Note

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor  $k=2$ , providing a level of confidence approximately 95 %.

Approved By :



Mr. Noppadon Luangart

Technical Manager

Issue Date :

19 August 2024

**เอกสารไม่ควบคุม**

## Calibration Note

UUC Adjustment : Not Adjust

Certificate No : 24-TPM-371

Request No : Req-2024-1693

Page : 2/2

## Result of Calibration :

UUC Sensor	Standard Temperature (°C)	UUC Reading (°C)	Correction (°C)	Uncertainty (± °C)
WET	20.031	20.0	0.0	0.13
	25.031	25.1	- 0.1	0.13
	30.034	30.0	0.0	0.13
	35.036	35.0	0.0	0.13
	40.035	40.0	0.0	0.13
	45.038	45.2	- 0.2	0.13
	50.041	50.0	0.0	0.13
	60.046	60.0	0.0	0.13
DRY	20.032	19.9	+ 0.1	0.13
	25.031	25.1	- 0.1	0.13
	30.034	29.9	+ 0.1	0.13
	35.036	35.1	- 0.1	0.13
	40.037	39.9	+ 0.1	0.13
	45.038	45.1	- 0.1	0.13
	50.041	48.9	+ 1.1	0.13
	60.046	59.9	+ 0.1	0.13
GLOBE	20.032	19.9	+ 0.1	0.13
	25.030	25.2	- 0.2	0.13
	30.035	29.9	+ 0.1	0.13
	35.035	35.1	- 0.1	0.13
	40.037	39.9	+ 0.1	0.13
	45.040	45.1	- 0.1	0.13
	50.040	50.0	0.0	0.13
	60.045	60.0	0.0	0.13

End of Certificate

Calibrated By :



Mr. Sittichok Jirapukdeesakul

เอกสารไม่ควบคุม



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)  
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES  
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250  
TEL. 0-2717-3000 29 FAX. 0-2719-9484



Cert.No.: 24CH239  
Page.: 1 of 3

## Certificate of Calibration

**Equipment :** pH Meter  
**Manufacturer :** Horiba  
**Model :** LAQUA-PH210  
**Serial No. :** HA0D0078  
**ID No. :** UAE.EFM.073/2564(EFM.pH.06/64)  
**Condition As-Received:** Used item  
**Received Date :** 19 February 2024  
**Calibration Date :** 20 February 2024  
**Reference :** 2402-0594WSC-3  
**Submitted by :** United Analyst and Engineering Consultant Co.,Ltd.  
3 Soi Udomsuk 41, Sukhumvit Road, Bangchak,  
Phrakhanong, Bangkok 10260  
**Ambient Temperature :** (25 ± 2.5) °C  
**Relative Humidity :** (50 ± 15) %  
**Calibration Procedure :** In - house method :  
- CP-CH5 by direct measurement with  
DC Voltage Standard and direct measurement  
with certified reference material (CRM)  
- CP-CH8 by comparison with temperature standard

**Calibrated by :** Walalak Sirithean

**Approved by :**

  
Approved Signatory

- ( ) Pornthippa Tameyakul  
( ) Unnopphol Harachai  
(✓) Saithip Meangmai

**Issue Date :** 22 February 2024

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written  
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

เอกสารไม่ควบคุม

A 0063841





Cert.No.: 24CH239

Page.: 2 of 3

**Condition of this calibration result**

**1. Reference Standard Instrument**

<u>Instrument</u>	<u>Serial No.</u>	<u>ID No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
1) Document Process Calibrator	54030049	130RC116	23E2802	27 Aug 2024
2) Ref. Standard Thermometer	4982054	110RC044	23I908	26 July 2024

This certification is traceable to the International System of Unit maintained through:-

- Technology Promotion Association (Thailand-Japan)

**2. Certified Reference Materials** : The measurement results are traceable to SI through CPA chem Ltd.,  
ANSI-ASQ National Accreditation Board, Accredited No. AR-1835

<u>Buffer Solution</u>	<u>Manufacturer</u>	<u>Lot No.</u>	<u>Exp. date</u>
pH 4.008	CPA chem	940102	27 Nov 2025
pH 6.986	CPA chem	940104	02 Nov 2024
pH 9.997	CPA chem	940106	02 Nov 2024

**3. This certificate is valid only to the item calibrated on date and place of calibration.**

**Calibration Results**

**Function : mV Measurement**

**Performing standard curve by Document Process Calibrator at pH (4,7)(7,10)**

Unit Under Calibration	Nominal Value	Standard Voltage Input	Actual Reading		Uncertainty of Measurement ( ±mV )	Coverage factor k
	pH	mV	mV	pH		
pH Meter S/N.: HA0D0078	4.00	177.48	177.4	4.01	0.058	2.00
	7.00	0.00	0.0	7.00	0.058	2.00
	7.00	0.00	0.0	7.00	0.058	2.00
	10.00	-177.48	-177.5	10.01	0.058	2.00

เอกสารไม่ควบคุม

a 1203292





Cert.No.: 24CH239

Page.: 3 of 3

**Calibration Results****Function : pH Measurement**

Performing three buffers standard curve by using buffer nominal pH (4,7)(7,10)

Unit Under Calibration	Standard pH Buffer Solution	Actual pH Reading	Actual mV Reading (mV)	Uncertainty of pH Measurement ( $\pm$ )	Coverage factor $k$
pH Electrode S/N.: 992H0385	4.008	4.02	168.3	0.0086	2.05
	6.986	6.99	-7.7	0.0093	2.00
	6.986	6.99	-7.6	0.011	2.00
	9.997	10.01	-180.7	0.0085	2.00

**Function : Temperature Measurement****(\*) Without adjustment**

This equipment was connected with Temperature Probe;

- Model : 9652

- Serial No. : 992H0385

Dimension of probe

- Length : 110 mm.

- Diameter : 16 mm.

- Immersion Depth : 100 mm.

Calibration Point ( $^{\circ}\text{C}$ )	Standard Temperature ( $^{\circ}\text{C}$ )	UUC* Reading ( $^{\circ}\text{C}$ )	Error ( $^{\circ}\text{C}$ )	Uncertainty of measurement ( $\pm$ $^{\circ}\text{C}$ )	Coverage factor $k$
25.0	25.000	25.0	0.000	0.13	2.00
30.0	30.000	30.0	0.000	0.13	2.00
35.0	34.999	35.0	0.001	0.13	2.00

**Remark** - UUC\* = Unit Under CalibratorThe reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor  $k$ , providing a level of confidence of approximately 95 %.

-o0o-

เอกสารไม่ควบคุม

a 1203291

## Certificate of Calibration

### Customer

Name : UNITED ANALYST AND ENGINEERING  
CONSULTANT CO.,LTD.  
Address : 81 Soi Udomsuk 41, Sukhumvit Road, Bangchak,  
Prakanong, Bangkok 10260

Certificate No : 24-ACT-091  
Request No : Req-2024-1380

### Unit Under Calibration Details

Measurement item : Acoustic Calibrator Class : 1  
Manufacturer : SVANTEK Range : 94 , 114 dB / 1000 Hz  
Model : SV 36 Instrument Status : Used  
Serial Number : 107224  
ID : UAE.EFM.171/2564

### Calibration Environment and Details


Temperature : ( 23 ±2 °C )  
Humidity : ( 50 ± 20 %RH )  
Barometric Pressure : ( 1013 ±10.0 hPa )  
Received Date : 24 June 2024  
Calibration Date : 26 June 2024  
Location of Calibration : LAB 1 Acoustic  
Calibration Procedure : In-house method CP-ACT-02 based on IEC 60942:2017 Electroacoustics - Sound calibrators


Reference Standard	Model	Serial Number	Traceable	Due Calibration
Sound Calibrator	SV 35A	58079	EEI	12 June 2025
THD Multimeter	2015	1047765	NIMT	16 January 2025

**Traceability** : This certificate provides traceability of measurement to recognized national standard, and to the realization of the international System of Units (SI).

### Note

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor  $k=2$ , providing a level of confidence approximately 95 %.

Calibrated By :   
Mr. Noppadon Luangart  
Service Calibration Engineer

Approved By :   
Mr. Pacit Mathavorn  
Calibration Engineer Supervisor

Issue Date : 26 June 2024

Certificate No : 24-ACT-091

Request No : Req-2024-1380

Sound pressure level

Calibration Results : Without Adjustment

Calibration Range (dB)	Without Adjustment (dB)		Adjustment (dB)		Uncertainty ( ± dB)	Acceptance limit Class 1 ( ± dB)	Result
	Measured	Deviated value	Measured	Deviated value			
94 dB / 1000 Hz	94.02	0.02	-	-	0.14	0.25	Pass
114 dB / 1000 Hz	114.05	0.05	-	-	0.13	0.25	Pass

Frequency of Sound pressure level

Calibration Range (Hz)	Without Adjustment		Adjustment		Uncertainty ( ± %)	Acceptance limit Class 1 ( ± %)	Result
	Measured (Hz)	Deviated	Measured (Hz)	Deviated			
94 dB / 1000 Hz	1000.00	0.00	-	-	0.01	0.70	Pass
114 dB / 1000 Hz	1000.00	0.00	-	-	0.01	0.70	Pass

Total Harmonic Distortion plus Noise of Sound pressure level (THD+N %)

Calibration Range (Hz)	Without Adjustment	Adjustment	Uncertainty ( ± %)	Acceptance limit Class 1 ( ± %)	Result
	Measured (%)	Measured (%)			
94 dB / 1000 Hz	0.24	-	0.40	2.5	Pass
114 dB / 1000 Hz	0.44	-	0.40	2.5	Pass

Note :

Function	Maximum-permitted Uncertainty of measurement
Sound pressure level	0.15 dB
Frequency	0.20%
Total distortion+noise	0.50%

- Acceptance limit was IEC60942:2017 Class 1

- The calibration results exclude the calibrator pressure correction

- The calibration results exclude the microphone volume correction

Certificate No : 24-ACT-091

Request No : Req-2024-1380

### Decision Rule for Statements of Conformity


The standard decision rule employed for the statements of conformity to each calibration result will be applied using ILAC-G8:09:2019, Guidelines on the Reporting of Compliance with Specification as following Fig. and statements

Pass = The measurement result plus the expanded uncertainty with a 95% coverage probability were within the limit.

Pass<sup>1</sup> = The measurement result was within the limit. However, a portion of the expanded uncertainty of measurement at 95% exceeds the limit.

Fail<sup>1</sup> = The measurement result was out of the limit. However, a portion of the expanded uncertainty of measurement at 95% is within the limit.

Fail = The measurement result plus the expanded uncertainty with a 95% coverage probability were outside the limit.

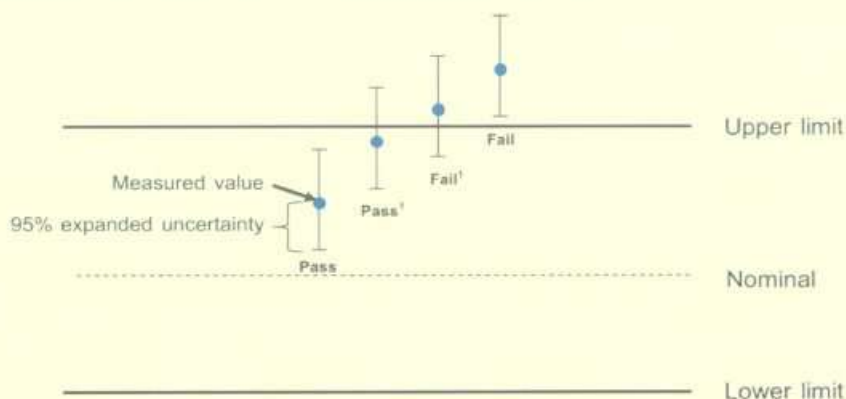

End of Calibration



Cert. No. : ACL24060

Pages : 1 of 8

## Calibration Certificate

**Equipment :** SOUND LEVEL METER  
**Manufacturer :** RION  
**Model :** NL-42 / Microphone UC-52 / Preamplifier NH-24  
**Serial No.:** 00709655 / 188530 / 01206  
**ID No.:** UAE.EFM.020/2564

**Condition As Found :** GOOD

**Customer :** UNITED ANALYST AND ENGINEERING CONSULTANT (UAE)  
81 SOI UDOMSUK 41, SUKHUMVIT ROAD,  
BANGCHAK SUB-DISTRICT,  
PHRAKHANONG DISTRICT, BANGKOK 10260  
THAILAND.

**Location :** -

**Ambient Temperature :** ( 23.0  $\pm$  3 ) °C  
**Pressure :** ( 101.3  $\pm$  3 ) kPa  
**Relative Humidity :** ( 50.0  $\pm$  20 ) %

**Received Date :** 21 DECEMBER 2023  
**Calibration Date :** 18-19 JANUARY 2024  
**Date of Issue :** 22 JANUARY 2024

**Calibrated by :**

Nathakorn Pisutpaisan

**Approved by :**

*T. Petchurai*  
( Thanakul Petchurai )

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

เอกสารไม่ควบคุม

# SITHIPORN ASSOCIATES CO., LTD. CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand  
Tel. +66 2433 8331 Email : calibration@sithiporn.com

SITHIPORN  
associates



Cert. No. : ACL24060  
Job No. : VC67AC0034  
Pages : 2 of 8

**Calibration Procedure :** CP-AC-01

## Calibration Method :

This equipment was calibrated by follow on IEC-61672-3 (2013) Standard for sound level meter (SLM).

The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.

For tests results of each items were made by observation of each Instruments display and also with SLM's display.

## Condition of this result of calibration :

### 1. Reference Standard Instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
Waveform Generator	33210A	MY48017076	EF-0009-23	07-FEB-24
Waveform Generator	33511B	MY52302742	EF-0010-23	07-FEB-24
Digital Multimeter	33461A	MY53220104	EEL.BP 30/0266	13-FEB-24
Digital Multimeter	33461A	MY53220076	EEL.BP 29/0266	13-FEB-24
Digital Multimeter	34461A	MY60024273	EEL.BP 31/0266	14-FEB-24
Programmable Attenuator	MAT-1070	62100114	EF-0011-23	08-FEB-24
Condenser Microphone	4180	2977900	AA-1001-23	14-FEB-24
Measuring Amplifier	NA-42KAI	34560495	AA-3002-23	14-FEB-24

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is traceable to the international system of unit maintained at :

3.1 National Institute of Metrology (Thailand).

3.2 Thailand Institute of Scientific and Technological Research (TISTR).

เอกสารไม่ควบคุม  
9. Kelen

# SITHIPORN ASSOCIATES CO., LTD. CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbunru, Bangplud, Bangkok, 10700 Thailand  
Tel. +66 2433 8331 Email : calibration@sithiporn.com

SITHIPORN  
associates



Cert. No. : ACL24060  
Job No. : VC67AC0034  
Pages : 3 of 8

## Summary of Measurement Result :

Parameter	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	0.2	N/A
2. Self-generated noise	0.2	N/A
3. Acoustical signal tests of frequency weightings		
125 Hz	0.3	0.6
1000 Hz	0.3	0.6
8000 Hz	0.3	0.7
4. Electrical signal tests of frequency weightings		
For 10 Hz to 4 kHz	0.3	0.6
For > 4 kHz to 10 kHz	0.3	0.7
For > 10 kHz to 20 kHz	-	1.0
5. Frequency and time weightings at 1 kHz	0.2	0.2
6. Long - term stability	0.1	0.1
7. Level linearity on the reference level range	0.2	0.3
8. Level linearity including the level range control	0.2	0.3
9. Tone burst response	0.2	0.3
10. Peak C sound level	0.2	0.35
11. Overload indication	0.2	0.25
12. High level stability	0.1	0.1

เอกสารไม่ควบคุม  
*T. Ketur*

**Cert. No. : ACL24060**

**Job No. : VC67AC0034**

**Pages : 4 of 8**

**Result of calibration :**

**1. Absolute sensitivity**

Reference Acoustic Signal ( dB )	Measured Value ( dB )	Deviation ( dB )	Acceptance Limit ( dB )
93.9 (93.98)	93.9	0.0	±0.3

**2. Self-generated noise**

**2.1 Normal test**

Measured Value ( dB )
15.1

**2.2 The microphone of the sound level meter was replaced by electrical signal input device.**

Frequency Weighting	Measured value ( dB )
A - weight	11.6
C - weight	17.5
Flat	23.3

**3. Acoustical signal tests of frequency weightings**

Meter free-field acoustic response at a level of 84 dB

Frequency ( Hz )	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
125	0.2	0.2	0.2	± 1.5
1000	0.1	0.1	0.1	± 1.0
8000	2.1	2.2	2.2	±5.0

**เอกสารไม่ควบคุม**  
*T. Kethan*



**Cert. No. : ACL24060**  
**Job No. : VC67AC0034**  
**Pages : 5 of 8**

#### 4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency ( Hz )	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	-0.1	-0.1	0.0	±2.0
125	0.0	0.0	0.0	±1.5
250	0.0	0.0	0.0	±1.5
500	0.0	0.0	0.0	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.0	0.0	±2.0
4000	0.0	0.0	0.0	±3.0
8000	0.0	0.1	0.1	±5.0

#### 5. Frequency and time weightings at 1 kHz

##### 5.1 Frequency weightings at 1 kHz

Frequency Weighting	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	94.0	94.0	0.0	± 0.2
C - weight	94.0	94.0	0.0	± 0.2
Flat	94.0	94.0	0.0	± 0.2

##### 5.2 Time weighting at 1 kHz

Frequency Weighting	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Fast	94.0	94.0	0.0	± 0.1
Slow	94.0	94.0	0.0	± 0.1
Leq	94.0	94.0	0.0	± 0.1

#### 6. Long - term stability

Frequency Weighting	SLM Display at initial ( dB )	SLM Display at final ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	94.0	94.0	0.0	± 0.3

เอกสารไม่ควบคุม  
 T. Kellern

# SITHIPORN ASSOCIATES CO., LTD. CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbunru, Bangplud, Bangkok, 10700 Thailand  
Tel. +66 2433 8331 Email : calibration@sithiporn.com

SITHIPORN  
associates



Cert. No. : ACL24060

Job No. : VC67AC0034

Pages : 6 of 8

## 7. Level linearity on the reference level range

Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
137.0	137.0	0.0	± 1.1
136.0	136.0	0.0	± 1.1
135.0	135.0	0.0	± 1.1
134.0	134.0	0.0	± 1.1
133.0	133.0	0.0	± 1.1
132.0	132.0	0.0	± 1.1
131.0	131.0	0.0	± 1.1
129.0	129.0	0.0	± 1.1
124.0	124.0	0.0	± 1.1
119.0	119.0	0.0	± 1.1
114.0	114.0	0.0	± 1.1
109.0	109.0	0.0	± 1.1
104.0	104.0	0.0	± 1.1
99.0	99.0	0.0	± 1.1
94.0	94.0	0.0	± 1.1
89.0	89.0	0.0	± 1.1
84.0	84.0	0.0	± 1.1
79.0	79.0	0.0	± 1.1
74.0	74.0	0.0	± 1.1
69.0	69.0	0.0	± 1.1
64.0	64.0	0.0	± 1.1
59.0	59.0	0.0	± 1.1
54.0	53.9	-0.1	± 1.1
49.0	49.0	0.0	± 1.1
44.0	44.0	0.0	± 1.1
39.0	38.9	-0.1	± 1.1
34.0	33.9	-0.1	± 1.1
30.0	29.9	-0.1	± 1.1
29.0	28.9	-0.1	± 1.1
28.0	27.9	-0.1	± 1.1
27.0	26.9	-0.1	± 1.1
26.0	25.9	-0.1	± 1.1
25.0	24.9	-0.1	± 1.1

เอกสารไม่ควบคุม  
*G. Kelen*

**Cert. No. : ACL24060**  
**Job No. : VC67AC0034**  
**Pages : 7 of 8**

**8. Level linearity including the level range control**

Range	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Auto	94.0	94.0	0.0	±1.1

**9. Tone burst response**

Time Weighting	Tone burst duration, Tb ( ms )	Cycle	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.0	0.0	±1.0
Slow	2	8	108.0	108.0	0.0	1.5 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
SEL	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.1	0.1	±1.0

**10. Peak C sound level**

Number of cycle in test signal	Anticipated Value ( dB )	Measured Value, Lcpeak ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Continuous	133.0	133.0	0.0	±3.0
One	136.4	136.2	-0.2	±3.0

Number of cycle in test signal	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Continuous	133.0	133.0	0.0	±2.0
Positive half cycle	135.4	135.2	-0.2	±2.0
Negative half cycle	135.4	135.2	-0.2	±2.0

**เอกสารไม่ควบคุม**  
*G. Petch*

# SITHIPORN ASSOCIATES CO., LTD. CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbunru, Bangplud, Bangkok, 10700 Thailand  
Tel. +66 2433 8331 Email : calibration@sithiporn.com

SITHIPORN  
associates



Cert. No. : ACL24060  
Job No. : VC67AC0034  
Pages : 8 of 8

## 11. Overload indication

Measured value ( dB )		Deviated Value ( dB )	Acceptance Limits ( dB )
Positive one-half cycle	Negative one-half cycle		
89.6	89.6	0.0	±1.5

## 12. High level stability

Frequency Weighting	SLM Display at initial ( dB )	SLM Display at final ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor  $k = 2$   
or any value following calculation, providing a level of confidence of approximately 95 %

End of Calibration Certificate

เอกสารไม่ควบคุม  
7. Kela



Cert. No. : ACL24166

Pages : 1 of 8

## Calibration Certificate

**Equipment :** SOUND LEVEL METER  
**Manufacturer :** RION  
**Model :** NL-42 / Microphone UC-52 / Preamplifier NH-24  
**Serial No.:** 01010782 / 194537 / 14660  
**ID No.:** UAE.EFM.083/2565

**Condition As Found :** GOOD

**Customer :** UNITED ANALYST AND ENGINEERING CONSULTANT (UAE)  
81 SOI UDOMSUK 41, SUKHUMVIT ROAD,  
BANGCHAK SUB-DISTRICT,  
PHRAKHANONG DISTRICT, BANGKOK 10260  
THAILAND.

**Location :** -

**Ambient Temperature :** ( 23.0  $\pm$  3 ) °C  
**Pressure :** ( 101.3  $\pm$  3 ) kPa  
**Relative Humidity :** ( 50.0  $\pm$  20 ) %

**Received Date :** 15 MAY 2024  
**Calibration Date :** 06 - 07 JUNE 2024  
**Date of Issue :** 07 JUNE 2024

**Calibrated by :**

Nathakorn Pisutpaisan

**Approved by :**

  
( Thanakul Petchurai )

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

เอกสารไม่ควบคุม

# SITHIPORN ASSOCIATES CO., LTD. CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand  
Tel. +66 2433 8331 Email : calibration@sithiporn.com

SITHIPORN  
associates



Cert. No. : ACL24166  
Job No. : VC67AC0090  
Pages : 2 of 8

Calibration Procedure : CP-AC-01

## Calibration Method :

This equipment was calibrated by follow on IEC-61672-3 (2013) Standard for sound level meter (SLM).

The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.

For tests results of each items were made by observation of each Instruments display and also with SLM's display.

## Condition of this result of calibration :

### 1. Reference Standard Instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
Waveform Generator	33210A	MY48017076	EF-0009-24	05-FEB-25
Waveform Generator	33511B	MY52302742	EF-0007-24	05-FEB-25
Digital Multimeter	33461A	MY53220104	EEL.BP 21/0267	13-FEB-25
Digital Multimeter	33461A	MY53220076	EEL.BP 20/0267	15-FEB-25
Digital Multimeter	34461A	MY60024273	EEL.BP 22/0267	15-FEB-25
Programmable Attenuator	MAT-1070	62100114	EF-0008-24	05-FEB-25
Condenser Microphone	4180	2977900	AA-1001-24	12-FEB-25
Measuring Amplifier	NA-42KAI	34560495	AA-3001-24	05-FEB-25

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is traceable to the international system of unit maintained at :

3.1 National Institute of Metrology (Thailand).

3.2 Thailand Institute of Scientific and Technological Research (TISTR).

เอกสารไม่ควบคุม

# SITHIPORN ASSOCIATES CO., LTD. CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand  
Tel. +66 2433 8331 Email : calibration@sithiphorn.com

SITHIPORN  
associates



Cert. No. : ACL24166  
Job No. : VC67AC0090  
Pages : 3 of 8

## Summary of Measurement Result :

Parameter	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	0.2	N/A
2. Self-generated noise	0.2	N/A
3. Acoustical signal tests of frequency weightings		
125 Hz	0.3	0.6
1000 Hz	0.3	0.6
8000 Hz	0.3	0.7
4. Electrical signal tests of frequency weightings		
For 10 Hz to 4 kHz	0.3	0.6
For > 4 kHz to 10 kHz	0.3	0.7
For > 10 kHz to 20 kHz	-	1.0
5. Frequency and time weightings at 1 kHz	0.2	0.2
6. Long - term stability	0.1	0.1
7. Level linearity on the reference level range	0.2	0.3
8. Level linearity including the level range control	0.2	0.3
9. Tone burst response	0.2	0.3
10. Peak C sound level	0.2	0.35
11. Overload indication	0.2	0.25
12. High level stability	0.1	0.1

เอกสารไม่ควบคุม  
T. Kewin

Cert. No. : ACL24166

Job No. : VC67AC0090

Pages : 4 of 8

**Result of calibration :**

**1. Absolute sensitivity**

Reference Acoustic Signal ( dB )	Measured Value ( dB )	Deviation ( dB )	Acceptance Limit ( dB )
93.9 (93.94)	93.9	0.0	±0.3

**2. Self-generated noise**

**2.1 Normal test**

Measured Value ( dB )
14.4

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Measured value ( dB )
A - weight	9.9
C - weight	16.6
Flat	22.4

**3. Acoustical signal tests of frequency weightings**

Meter free-field acoustic response at a level of 84 dB

Frequency ( Hz )	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
125	0.1	0.2	0.2	± 1.5
1000	-0.1	-0.1	-0.1	± 1.0
8000	0.2	0.3	0.2	±5.0



**Cert. No. : ACL24166**  
**Job No. : VC67AC0090**  
**Pages : 5 of 8**

#### 4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency ( Hz )	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	-0.1	-0.1	0.0	±2.0
125	0.0	0.0	0.0	±1.5
250	0.0	0.0	-0.1	±1.5
500	0.0	0.0	-0.1	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.0	0.0	±2.0
4000	0.0	0.0	0.0	±3.0
8000	0.0	0.1	0.1	±5.0

#### 5. Frequency and time weightings at 1 kHz

##### 5.1 Frequency weightings at 1 kHz

Frequency Weighting	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	94.0	94.0	0.0	± 0.2
C - weight	94.0	94.0	0.0	± 0.2
Flat	94.0	94.0	0.0	± 0.2

##### 5.2 Time weighting at 1 kHz

Frequency Weighting	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Fast	94.0	94.0	0.0	± 0.1
Slow	94.0	94.0	0.0	± 0.1
Leq	94.0	94.0	0.0	± 0.1

#### 6. Long - term stability

Frequency Weighting	SLM Display at initial ( dB )	SLM Display at final ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	94.0	94.0	0.0	

เอกสารไม่ควบคุม

*T. Rekh*

# SITHIPORN ASSOCIATES CO., LTD. CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand  
Tel. +66 2433 8331 Email : calibration@sithiphorn.com

SITHIPORN  
associates



Cert. No. : ACL24166

Job No. : VC67AC0090

Pages : 6 of 8

## 7. Level linearity on the reference level range

Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
137.0	137.0	0.0	$\pm 1.1$
136.0	136.0	0.0	$\pm 1.1$
135.0	135.0	0.0	$\pm 1.1$
134.0	134.0	0.0	$\pm 1.1$
133.0	133.0	0.0	$\pm 1.1$
132.0	132.0	0.0	$\pm 1.1$
131.0	131.0	0.0	$\pm 1.1$
129.0	129.0	0.0	$\pm 1.1$
124.0	124.0	0.0	$\pm 1.1$
119.0	119.0	0.0	$\pm 1.1$
114.0	114.0	0.0	$\pm 1.1$
109.0	109.0	0.0	$\pm 1.1$
104.0	104.0	0.0	$\pm 1.1$
99.0	99.0	0.0	$\pm 1.1$
94.0	94.0	0.0	$\pm 1.1$
89.0	89.1	0.1	$\pm 1.1$
84.0	84.0	0.0	$\pm 1.1$
79.0	79.0	0.0	$\pm 1.1$
74.0	74.1	0.1	$\pm 1.1$
69.0	69.1	0.1	$\pm 1.1$
64.0	64.0	0.0	$\pm 1.1$
59.0	59.1	0.1	$\pm 1.1$
54.0	54.0	0.0	$\pm 1.1$
49.0	49.0	0.0	$\pm 1.1$
44.0	44.0	0.0	$\pm 1.1$
39.0	39.0	0.0	$\pm 1.1$
34.0	34.0	0.0	$\pm 1.1$
30.0	30.0	0.0	$\pm 1.1$
29.0	29.0	0.0	$\pm 1.1$
28.0	28.0	0.0	$\pm 1.1$
27.0	27.0	0.0	$\pm 1.1$
26.0	26.0	0.0	$\pm 1.1$
25.0	25.0	0.0	$\pm 1.1$

เอกสารไม่ควบคุม  
7. Kelen.

**Cert. No. : ACL24166**  
**Job No. : VC67AC0090**  
**Pages : 7 of 8**

**8. Level linearity including the level range control**

Range	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Auto	94.0	94.0	0.0	±1.1

**9. Tone burst response**

Time Weighting	Tone burst duration, Tb ( ms )	Cycle	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.0	0.0	±1.0
Slow	2	8	108.0	108.0	0.0	1.5 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
SEL	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.0	0.0	±1.0

**10. Peak C sound level**

Number of cycle in test signal	Anticipated Value ( dB )	Measured Value, Lcpeak ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Continuous	133.0	133.0	0.0	±3.0
One	136.4	136.4	0.0	±3.0

Number of cycle in test signal	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Continuous	133.0	133.1	0.1	±2.0
Positive half cycle	135.4	135.3	-0.1	±2.0
Negative half cycle	135.4	135.3	-0.1	±2.0

**เอกสารไม่ควบคุม**  
*J. Kell...*

# SITHIPORN ASSOCIATES CO., LTD. CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand  
Tel. +66 2433 8331 Email : calibration@sithiporn.com

SITHIPORN  
associates



Cert. No. : ACL24166  
Job No. : VC67AC0090  
Pages : 8 of 8

## 11. Overload indication

Measured value ( dB )		Deviated Value ( dB )	Acceptance Limits ( dB )
Positive one-half cycle	Negative one-half cycle		
89.6	89.6	0.0	±1.5

## 12. High level stability

Frequency Weighting	SLM Display at initial ( dB )	SLM Display at final ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor  $k = 2$   
or any value following calculation, providing a level of confidence of approximately 95 %

————— **End of Calibration Certificate** —————

เอกสารไม่ควบคุม  
*T. Kelen*



Cert. No. : ACL24098

Pages : 1 of 8

## Calibration Certificate

**Equipment :** SOUND LEVEL METER  
**Manufacturer :** RION  
**Model :** NL-42 / Microphone UC-52 / Preamplifier NH-24  
**Serial No.:** 00408981 / 186171 / 90426  
**ID No.:** UAE.EFM.008/2564

**Condition As Found :** GOOD

**Customer :** UNITED ANALYST AND ENGINEERING CONSULTANT (UAE)  
81 SOI UDOMSUK 41, SUKHUMVIT ROAD,  
BANGCHAK SUB-DISTRICT,  
PHRAKHANONG DISTRICT, BANGKOK 10260  
THAILAND.

**Location :** -  
**Ambient Temperature :** ( 23.0  $\pm$  3 ) °C  
**Pressure :** ( 101.3  $\pm$  3 ) kPa  
**Relative Humidity :** ( 50.0  $\pm$  20 ) %

**Received Date :** 18 JANUARY 2024  
**Calibration Date :** 29-30 JANUARY 2024  
**Date of Issue :** 02 FEBRUARY 2024

**Calibrated by :** Nathakorn Pisutpaisan

**Approved by :**

  
( Thanakul Petchurai )

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

เอกสารไม่ควบคุม

# SITHIPORN ASSOCIATES CO., LTD.

## CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand  
Tel. +66 2433 8331 Email : calibration@sithiporn.com



Cert. No. : ACL24098  
Job No. : VC67AC0057  
Pages : 2 of 8

Calibration Procedure : CP-AC-01

### Calibration Method :

This equipment was calibrated by follow on IEC-61672-3 (2013) Standard for sound level meter (SLM).

The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.

For tests results of each items were made by observation of each Instruments display and also with SLM's display.

### Condition of this result of calibration :

#### 1. Reference Standard Instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
Waveform Generator	33210A	MY48017076	EF-0009-23	07-FEB-24
Waveform Generator	33511B	MY52302742	EF-0010-23	07-FEB-24
Digital Multimeter	33461A	MY53220104	EEL.BP 30/0266	13-FEB-24
Digital Multimeter	33461A	MY53220076	EEL.BP 29/0266	13-FEB-24
Digital Multimeter	34461A	MY60024273	EEL.BP 31/0266	14-FEB-24
Programmable Attenuator	MAT-1070	62100114	EF-0011-23	08-FEB-24
Condenser Microphone	4180	2977900	AA-1001-23	14-FEB-24
Measuring Amplifier	NA-42KAI	34560495	AA-3002-23	14-FEB-24

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is traceable to the international system of unit maintained at :

3.1 National Institute of Metrology (Thailand).

3.2 Thailand Institute of Scientific and Technological Research (TISTR).

เอกสารไม่ควบคุม  
*[Signature]*

# SITHIPORN ASSOCIATES CO., LTD.

## CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand  
Tel. +66 2433 8331 Email : calibration@sithiporn.com

SITHIPORN  
associates



Cert. No. : ACL24098

Job No. : VC67AC0057

Pages : 3 of 8

### Summary of Measurement Result :

Parameter	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	0.2	N/A
2. Self-generated noise	0.2	N/A
3. Acoustical signal tests of frequency weightings		
125 Hz	0.3	0.6
1000 Hz	0.3	0.6
8000 Hz	0.3	0.7
4. Electrical signal tests of frequency weightings		
For 10 Hz to 4 kHz	0.3	0.6
For > 4 kHz to 10 kHz	0.3	0.7
For > 10 kHz to 20 kHz	-	1.0
5. Frequency and time weightings at 1 kHz	0.2	0.2
6. Long - term stability	0.1	0.1
7. Level linearity on the reference level range	0.2	0.3
8. Level linearity including the level range control	0.2	0.3
9. Tone burst response	0.2	0.3
10. Peak C sound level	0.2	0.35
11. Overload indication	0.2	0.25
12. High level stability	0.1	0.1

เอกสารไม่ควบคุม  
T. Kech

# SITHIPORN ASSOCIATES CO., LTD.

## CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand  
Tel. +66 2433 8331 Email : calibration@sithiporn.com

SITHIPORN  
associates



Cert. No. : ACL24098

Job No. : VC67AC0057

Pages : 4 of 8

### Result of calibration :

#### 1. Absolute sensitivity

Reference Acoustic Signal ( dB )	Measured Value ( dB )	Deviation ( dB )	Acceptance Limit ( dB )
93.9 (93.98)	93.9	0.0	±0.3

#### 2. Self-generated noise

##### 2.1 Normal test

Measured Value ( dB )
14.6

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Measured value ( dB )
A - weight	10.8
C - weight	16.8
Flat	23.0

#### 3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency ( Hz )	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
125	0.5	0.5	0.5	± 1.5
1000	0.0	0.0	0.0	± 1.0
8000	1.0	1.0	1.0	±5.0

เอกสารไม่ควบคุม  
T. Kewin



**Cert. No. : ACL24098**  
**Job No. : VC67AC0057**  
**Pages : 5 of 8**

#### 4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency ( Hz )	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	0.0	-0.2	-0.1	±2.0
125	-0.1	0.0	-0.1	±1.5
250	0.0	-0.1	-0.1	±1.5
500	0.0	0.0	-0.1	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.0	0.0	±2.0
4000	0.0	0.0	0.0	±3.0
8000	0.0	0.0	0.0	±5.0

#### 5. Frequency and time weightings at 1 kHz

##### 5.1 Frequency weightings at 1 kHz

Frequency Weighting	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	94.0	94.0	0.0	± 0.2
C - weight	94.0	94.0	0.0	± 0.2
Flat	94.0	94.0	0.0	± 0.2

##### 5.2 Time weighting at 1 kHz

Frequency Weighting	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Fast	94.0	94.0	0.0	± 0.1
Slow	94.0	94.0	0.0	± 0.1
Leq	94.0	94.0	0.0	± 0.1

#### 6. Long - term stability

Frequency Weighting	SLM Display at initial ( dB )	SLM Display at final ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	94.0	94.0	0.0	± 0.3

เอกสารไม่ควบคุม  
 T. Kelen

# SITHIPORN ASSOCIATES CO., LTD.

## CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand  
Tel. +66 2433 8331 Email : calibration@sithiporn.com

SITHIPORN  
associates



Cert. No. : ACL24098

Job No. : VC67AC0057

Pages : 6 of 8

### 7. Level linearity on the reference level range

Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
137.0	137.1	0.1	± 1.1
136.0	136.1	0.1	± 1.1
135.0	135.1	0.1	± 1.1
134.0	134.1	0.1	± 1.1
133.0	133.0	0.0	± 1.1
132.0	132.0	0.0	± 1.1
131.0	131.0	0.0	± 1.1
129.0	129.1	0.1	± 1.1
124.0	124.0	0.0	± 1.1
119.0	119.1	0.1	± 1.1
114.0	114.1	0.1	± 1.1
109.0	109.1	0.1	± 1.1
104.0	104.1	0.1	± 1.1
99.0	99.1	0.1	± 1.1
94.0	94.0	0.0	± 1.1
89.0	89.0	0.0	± 1.1
84.0	84.0	0.0	± 1.1
79.0	79.0	0.0	± 1.1
74.0	74.0	0.0	± 1.1
69.0	69.0	0.0	± 1.1
64.0	64.0	0.0	± 1.1
59.0	59.0	0.0	± 1.1
54.0	54.0	0.0	± 1.1
49.0	49.0	0.0	± 1.1
44.0	44.0	0.0	± 1.1
39.0	39.0	0.0	± 1.1
34.0	34.0	0.0	± 1.1
30.0	29.9	-0.1	± 1.1
29.0	28.9	-0.1	± 1.1
28.0	27.9	-0.1	± 1.1
27.0	26.9	-0.1	± 1.1
26.0	25.9	-0.1	± 1.1
25.0	24.9	-0.1	± 1.1

เอกสารไม่ควบคุม  
7. Recheck -

**Cert. No. : ACL24098**  
**Job No. : VC67AC0057**  
**Pages : 7 of 8**

**8. Level linearity including the level range control**

Range	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Auto	94.0	94.0	0.0	±1.1

**9. Tone burst response**

Time Weighting	Tone burst duration, Tb ( ms )	Cycle	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.0	0.0	±1.0
Slow	2	8	108.0	108.0	0.0	1.5 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
SEL	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.0	0.0	±1.0

**10. Peak C sound level**

Number of cycle in test signal	Anticipated Value ( dB )	Measured Value, Lcpeak ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Continuous	133.0	133.0	0.0	±3.0
One	136.4	135.9	-0.5	±3.0

Number of cycle in test signal	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Continuous	133.0	133.0	0.0	±2.0
Positive half cycle	135.4	135.1	-0.3	±2.0
Negative half cycle	135.4	135.1	-0.3	±2.0

**เอกสารไม่ควบคุม**  
*7. K. K.*

# SITHIPORN ASSOCIATES CO., LTD.

## CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand  
Tel. +66 2433 8331 Email : calibration@sithiporn.com

SITHIPORN  
associates



Cert. No. : ACL24098  
Job No. : VC67AC0057  
Pages : 8 of 8

### 11. Overload indication

Measured value ( dB )		Deviated Value ( dB )	Acceptance Limits ( dB )
Positive one-half cycle	Negative one-half cycle		
89.5	89.5	0.0	±1.5

### 12. High level stability

Frequency Weighting	SLM Display at initial ( dB )	SLM Display at final ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor  $k = 2$   
or any value following calculation, providing a level of confidence of approximately 95 %

————— End of Calibration Certificate —————

เอกสารไม่ควบคุม  
*T. Ketch.*



Cert. No. : ACL24058

Pages : 1 of 8

## Calibration Certificate

**Equipment :** SOUND LEVEL METER  
**Manufacturer :** RION  
**Model :** NL-42 / Microphone UC-52 / Preamplifier NH-24  
**Serial No.:** 00609500 / 189689 / 01126  
**ID No.:** UAE.EFM.018/2564

**Condition As Found :** GOOD

**Customer :** UNITED ANALYST AND ENGINEERING CONSULTANT (UAE)  
81 SOI UDOMSUK 41, SUKHUMVIT ROAD,  
BANGCHAK SUB-DISTRICT,  
PHRAKHANONG DISTRICT, BANGKOK 10260  
THAILAND.

**Location :** -

**Ambient Temperature :** ( 23.0  $\pm$  3 ) °C  
**Pressure :** ( 101.3  $\pm$  3 ) kPa  
**Relative Humidity :** ( 50.0  $\pm$  20 ) %

**Received Date :** 21 DECEMBER 2023  
**Calibration Date :** 18-19 JANUARY 2024  
**Date of Issue :** 22 JANUARY 2024

**Calibrated by :**

Nathakorn Pisutpaisan

**Approved by :**

  
( Thanakul Petchurai )

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

เอกสารไม่ควบคุม

# SITHIPORN ASSOCIATES CO., LTD.

## CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbunru, Bangplud, Bangkok, 10700 Thailand  
Tel. +66 2433 8331 Email : calibration@sithiporn.com



Cert. No. : ACL24058  
Job No. : VC67AC0034  
Pages : 2 of 8

Calibration Procedure : CP-AC-01

### Calibration Method :

This equipment was calibrated by follow on IEC-61672-3 (2013) Standard for sound level meter (SLM).

The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.

For tests results of each items were made by observation of each Instruments display and also with SLM's display.

### Condition of this result of calibration :

#### 1. Reference Standard Instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
Waveform Generator	33210A	MY48017076	EF-0009-23	07-FEB-24
Waveform Generator	33511B	MY52302742	EF-0010-23	07-FEB-24
Digital Multimeter	33461A	MY53220104	EEL.BP 30/0266	13-FEB-24
Digital Multimeter	33461A	MY53220076	EEL.BP 29/0266	13-FEB-24
Digital Multimeter	34461A	MY60024273	EEL.BP 31/0266	14-FEB-24
Programmable Attenuator	MAT-1070	62100114	EF-0011-23	08-FEB-24
Condenser Microphone	4180	2977900	AA-1001-23	14-FEB-24
Measuring Amplifier	NA-42KAI	34560495	AA-3002-23	14-FEB-24

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is traceable to the international system of unit maintained at :

3.1 National Institute of Metrology (Thailand).

3.2 Thailand Institute of Scientific and Technological Research (TISTR).

เอกสารไม่ควบคุม  
9. Kew

# SITHIPORN ASSOCIATES CO., LTD.

## CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand  
Tel. +66 2433 8331 Email : calibration@sithiporn.com

SITHIPORN  
associates



Cert. No. : ACL24058

Job No. : VC67AC0034

Pages : 3 of 8

### Summary of Measurement Result :

Parameter	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	0.2	N/A
2. Self-generated noise	0.2	N/A
3. Acoustical signal tests of frequency weightings		
125 Hz	0.3	0.6
1000 Hz	0.3	0.6
8000 Hz	0.3	0.7
4. Electrical signal tests of frequency weightings		
For 10 Hz to 4 kHz	0.3	0.6
For > 4 kHz to 10 kHz	0.3	0.7
For > 10 kHz to 20 kHz	-	1.0
5. Frequency and time weightings at 1 kHz	0.2	0.2
6. Long - term stability	0.1	0.1
7. Level linearity on the reference level range	0.2	0.3
8. Level linearity including the level range control	0.2	0.3
9. Tone burst response	0.2	0.3
10. Peak C sound level	0.2	0.35
11. Overload indication	0.2	0.25
12. High level stability	0.1	0.1

เอกสารไม่ควบคุม  
*G. Kewin*

# SITHIPORN ASSOCIATES CO., LTD.

## CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand  
Tel. +66 2433 8331 Email : calibration@sithiporn.com

SITHIPORN  
associates



Cert. No. : ACL24058

Job No. : VC67AC0034

Pages : 4 of 8

### Result of calibration :

#### 1. Absolute sensitivity

Reference Acoustic Signal ( dB )	Measured Value ( dB )	Deviation ( dB )	Acceptance Limit ( dB )
93.9 (93.98)	93.9	0.0	±0.3

#### 2. Self-generated noise

##### 2.1 Normal test

Measured Value ( dB )
18.2

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Measured value ( dB )
A - weight	14.4
C - weight	20.7
Flat	26.5

#### 3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency ( Hz )	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
125	0.0	0.0	0.0	± 1.5
1000	-0.1	-0.1	-0.1	± 1.0
8000	1.4	1.5	1.5	±5.0

เอกสารไม่ควบคุม  
7. Kellin



**Cert. No. : ACL24058**  
**Job No. : VC67AC0034**  
**Pages : 5 of 8**

#### 4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency ( Hz )	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	0.0	0.0	0.0	±2.0
125	0.1	0.1	0.0	±1.5
250	0.0	0.0	0.0	±1.5
500	0.0	0.1	0.0	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.1	0.0	±2.0
4000	0.0	0.0	0.0	±3.0
8000	0.0	0.1	0.1	±5.0

#### 5. Frequency and time weightings at 1 kHz

##### 5.1 Frequency weightings at 1 kHz

Frequency Weighting	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	94.0	94.0	0.0	± 0.2
C - weight	94.0	94.0	0.0	± 0.2
Flat	94.0	94.0	0.0	± 0.2

##### 5.2 Time weighting at 1 kHz

Frequency Weighting	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Fast	94.0	94.0	0.0	± 0.1
Slow	94.0	94.0	0.0	± 0.1
Leq	94.0	94.0	0.0	± 0.1

#### 6. Long - term stability

Frequency Weighting	SLM Display at initial ( dB )	SLM Display at final ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	94.0	94.0	0.0	± 0.3

เอกสารไม่ควบคุม

7. Kewin

# SITHIPORN ASSOCIATES CO., LTD.

## CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand  
Tel. +66 2433 8331 Email : calibration@sithiporn.com

SITHIPORN  
associates



Cert. No. : ACL24058

Job No. : VC67AC0034

Pages : 6 of 8

### 7. Level linearity on the reference level range

Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
137.0	137.0	0.0	$\pm 1.1$
136.0	136.0	0.0	$\pm 1.1$
135.0	135.0	0.0	$\pm 1.1$
134.0	134.0	0.0	$\pm 1.1$
133.0	133.0	0.0	$\pm 1.1$
132.0	132.0	0.0	$\pm 1.1$
131.0	131.0	0.0	$\pm 1.1$
129.0	129.0	0.0	$\pm 1.1$
124.0	124.0	0.0	$\pm 1.1$
119.0	119.0	0.0	$\pm 1.1$
114.0	114.0	0.0	$\pm 1.1$
109.0	109.0	0.0	$\pm 1.1$
104.0	104.0	0.0	$\pm 1.1$
99.0	99.0	0.0	$\pm 1.1$
94.0	94.0	0.0	$\pm 1.1$
89.0	89.0	0.0	$\pm 1.1$
84.0	84.0	0.0	$\pm 1.1$
79.0	79.0	0.0	$\pm 1.1$
74.0	74.0	0.0	$\pm 1.1$
69.0	69.0	0.0	$\pm 1.1$
64.0	64.0	0.0	$\pm 1.1$
59.0	59.0	0.0	$\pm 1.1$
54.0	54.0	0.0	$\pm 1.1$
49.0	49.0	0.0	$\pm 1.1$
44.0	44.0	0.0	$\pm 1.1$
39.0	39.0	0.0	$\pm 1.1$
34.0	34.1	0.1	$\pm 1.1$
30.0	30.1	0.1	$\pm 1.1$
29.0	29.2	0.2	$\pm 1.1$
28.0	28.2	0.2	$\pm 1.1$
27.0	27.3	0.3	$\pm 1.1$
26.0	26.4	0.4	$\pm 1.1$
25.0	25.5	0.5	$\pm 1.1$

เอกสารไม่ควบคุม  
7. Kelvin.

# SITHIPORN ASSOCIATES CO., LTD.

## CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand  
Tel, +66 2433 8331 Email : calibration@sithiporn.com

SITHIPORN  
associates



Cert. No. : ACL24058  
Job No. : VC67AC0034  
Pages : 7 of 8

### 8. Level linearity including the level range control

Range	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Auto	94.0	94.0	0.0	±1.1

### 9. Tone burst response

Time Weighting	Tone burst duration, Tb ( ms )	Cycle	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.1	0.1	±1.0
Slow	2	8	108.0	108.0	0.0	1.5 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
SEL	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.1	0.1	±1.0

### 10. Peak C sound level

Number of cycle in test signal	Anticipated Value ( dB )	Measured Value, Lcpeak ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Continuous	133.0	133.0	0.0	±3.0
One	136.4	136.3	-0.1	±3.0

Number of cycle in test signal	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Continuous	133.0	133.0	0.0	±2.0
Positive half cycle	135.4	135.1	-0.3	±2.0
Negative half cycle	135.4	135.1	-0.3	±2.0

เอกสารไม่ควบคุม  
7. Kewin

# SITHIPORN ASSOCIATES CO., LTD. CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbunru, Bangplud, Bangkok, 10700 Thailand  
Tel. +66 2433 8331 Email : calibration@sithiporn.com

SITHIPORN  
associates



Cert. No. : ACL24058

Job No. : VC67AC0034

Pages : 8 of 8

## 11. Overload indication

Measured value ( dB )		Deviated Value ( dB )	Acceptance Limits ( dB )
Positive one-half cycle	Negative one-half cycle		
89.6	89.5	-0.1	±1.5

## 12. High level stability

Frequency Weighting	SLM Display at initial ( dB )	SLM Display at final ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor  $k = 2$   
or any value following calculation, providing a level of confidence of approximately 95 %

————— End of Calibration Certificate —————

เอกสารไม่ควบคุม  
7. Kelen



Cert. No. : ACL24156

Pages : 1 of 8

## Calibration Certificate

**Equipment :** SOUND LEVEL METER  
**Manufacturer :** RION  
**Model :** NL-42 / Microphone UC-52 / Preamplifier NH-24  
**Serial No.:** 00321441 / 139083 / 11461  
**ID No.:** UAE.EMA2.090/2555

**Condition As Found :** GOOD

**Customer :** UNITED ANALYST AND ENGINEERING CONSULTANT (UAE)  
81 SOI UDOMSUK 41, SUKHUMVIT ROAD,  
BANGCHAK SUB-DISTRICT,  
PHRAKHANONG DISTRICT, BANGKOK 10260  
THAILAND.

**Location :** -

**Ambient Temperature :** ( 23.0  $\pm$  3 ) °C  
**Pressure :** ( 101.3  $\pm$  3 ) kPa  
**Relative Humidity :** ( 50.0  $\pm$  20 ) %

**Received Date :** 10 MAY 2024  
**Calibration Date :** 30 - 31 MAY 2024  
**Date of Issue :** 04 JUNE 2024

**Calibrated by :**

Nathakorn Pisutpaisan

**Approved by :**

  
( Thanakul Petchurai )

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

**เอกสารไม่ควบคุม**

# SITHIPORN ASSOCIATES CO., LTD.

## CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbunru, Bangplud, Bangkok, 10700 Thailand  
Tel. +66 2433 8331 Email : calibration@sithiporn.com



Cert. No. : ACL24156  
Job No. : VC67AC0071  
Pages : 2 of 8

Calibration Procedure : CP-AC-01

### Calibration Method :

This equipment was calibrated by follow on IEC-61672-3 (2013) Standard for sound level meter (SLM).

The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.

For tests results of each items were made by observation of each Instruments display and also with SLM's display.

### Condition of this result of calibration :

#### 1. Reference Standard Instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
Waveform Generator	33210A	MY48017076	EF-0009-24	05-FEB-25
Waveform Generator	33511B	MY52302742	EF-0007-24	05-FEB-25
Digital Multimeter	33461A	MY53220104	EEL.BP 21/0267	13-FEB-25
Digital Multimeter	33461A	MY53220076	EEL.BP 20/0267	15-FEB-25
Digital Multimeter	34461A	MY60024273	EEL.BP 22/0267	15-FEB-25
Programmable Attenuator	MAT-1070	62100114	EF-0008-24	05-FEB-25
Condenser Microphone	4180	2977900	AA-1001-24	12-FEB-25
Measuring Amplifier	NA-42KAI	34560495	AA-3001-24	05-FEB-25

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is traceable to the international system of unit maintained at :

3.1 National Institute of Metrology (Thailand).

3.2 Thailand Institute of Scientific and Technological Research (TISTR).

เอกสารไม่ควบคุม  
*G. Petch*

# SITHIPORN ASSOCIATES CO., LTD. CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand  
Tel. +66 2433 8331 Email : calibration@sithiporn.com

SITHIPORN  
associates



Cert. No. : ACL24156

Job No. : VC67AC0071

Pages : 3 of 8

## Summary of Measurement Result :

Parameter	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	0.2	N/A
2. Self-generated noise	0.2	N/A
3. Acoustical signal tests of frequency weightings		
125 Hz	0.3	0.6
1000 Hz	0.3	0.6
8000 Hz	0.3	0.7
4. Electrical signal tests of frequency weightings		
For 10 Hz to 4 kHz	0.3	0.6
For > 4 kHz to 10 kHz	0.3	0.7
For > 10 kHz to 20 kHz	-	1.0
5. Frequency and time weightings at 1 kHz	0.2	0.2
6. Long - term stability	0.1	0.1
7. Level linearity on the reference level range	0.2	0.3
8. Level linearity including the level range control	0.2	0.3
9. Tone burst response	0.2	0.3
10. Peak C sound level	0.2	0.35
11. Overload indication	0.2	0.25
12. High level stability	0.1	0.1

เอกสารไม่ควบคุม  
*T. Keth*

# SITHIPORN ASSOCIATES CO., LTD.

## CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand  
Tel. +66 2433 8331 Email : calibration@sithiporn.com

SITHIPORN  
associates



Cert. No. : ACL24156

Job No. : VC67AC0071

Pages : 4 of 8

### Result of calibration :

#### 1. Absolute sensitivity

Reference Acoustic Signal ( dB )	Measured Value ( dB )	Deviation ( dB )	Acceptance Limit ( dB )
93.9 (93.94)	93.9	0.0	±0.3

#### 2. Self-generated noise

##### 2.1 Normal test

Measured Value ( dB )
16.6

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Measured value ( dB )
A - weight	14.2
C - weight	20.2
Flat	26.0

#### 3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency ( Hz )	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
125	-0.2	-0.1	-0.1	± 1.5
1000	-0.2	-0.2	-0.2	± 1.0
8000	0.5	0.5	0.5	±5.0

เอกสารไม่ควบคุม  
*[Signature]*



**Cert. No. : ACL24156**  
**Job No. : VC67AC0071**  
**Pages : 5 of 8**

#### 4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency ( Hz )	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	-0.1	-0.1	-0.2	±2.0
125	-0.1	0.0	0.0	±1.5
250	-0.1	-0.1	-0.1	±1.5
500	0.0	0.0	-0.1	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.0	0.0	±2.0
4000	0.0	0.0	0.0	±3.0
8000	0.0	0.0	0.0	±5.0

#### 5. Frequency and time weightings at 1 kHz

##### 5.1 Frequency weightings at 1 kHz

Frequency Weighting	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	94.0	94.0	0.0	± 0.2
C - weight	94.0	94.0	0.0	± 0.2
Flat	94.0	94.0	0.0	± 0.2

##### 5.2 Time weighting at 1 kHz

Frequency Weighting	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Fast	94.0	94.0	0.0	± 0.1
Slow	94.0	94.0	0.0	± 0.1
Leq	94.0	94.0	0.0	± 0.1

#### 6. Long - term stability

Frequency Weighting	SLM Display at initial ( dB )	SLM Display at final ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	94.0	94.0	0.0	

**เอกสารไม่ควบคุม**

*J. Petch*

# SITHIPORN ASSOCIATES CO., LTD.

## CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand  
Tel, +66 2433 8331 Email : calibration@sithiporn.com

SITHIPORN  
associates



Cert. No. : ACL24156

Job No. : VC67AC0071

Pages : 6 of 8

### 7. Level linearity on the reference level range

Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
137.0	137.1	0.1	$\pm 1.1$
136.0	136.1	0.1	$\pm 1.1$
135.0	135.1	0.1	$\pm 1.1$
134.0	134.1	0.1	$\pm 1.1$
133.0	133.0	0.0	$\pm 1.1$
132.0	132.0	0.0	$\pm 1.1$
131.0	131.0	0.0	$\pm 1.1$
129.0	129.1	0.1	$\pm 1.1$
124.0	124.0	0.0	$\pm 1.1$
119.0	119.1	0.1	$\pm 1.1$
114.0	114.1	0.1	$\pm 1.1$
109.0	109.1	0.1	$\pm 1.1$
104.0	104.1	0.1	$\pm 1.1$
99.0	99.1	0.1	$\pm 1.1$
94.0	94.0	0.0	$\pm 1.1$
89.0	89.0	0.0	$\pm 1.1$
84.0	84.0	0.0	$\pm 1.1$
79.0	79.0	0.0	$\pm 1.1$
74.0	74.0	0.0	$\pm 1.1$
69.0	69.0	0.0	$\pm 1.1$
64.0	64.0	0.0	$\pm 1.1$
59.0	59.0	0.0	$\pm 1.1$
54.0	54.0	0.0	$\pm 1.1$
49.0	49.0	0.0	$\pm 1.1$
44.0	44.0	0.0	$\pm 1.1$
39.0	39.0	0.0	$\pm 1.1$
34.0	34.0	0.0	$\pm 1.1$
30.0	30.0	0.0	$\pm 1.1$
29.0	29.0	0.0	$\pm 1.1$
28.0	28.0	0.0	$\pm 1.1$
27.0	27.0	0.0	$\pm 1.1$
26.0	26.1	0.1	$\pm 1.1$
25.0	25.0	0.0	$\pm 1.1$

เอกสารไม่ควบคุม  
7. Ketch

**Cert. No. : ACL24156**  
**Job No. : VC67AC0071**  
**Pages : 7 of 8**

**8. Level linearity including the level range control**

Range	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Auto	94.0	94.0	0.0	±1.1

**9. Tone burst response**

Time Weighting	Tone burst duration, Tb ( ms )	Cycle	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.0	0.0	±1.0
Slow	2	8	108.0	108.0	0.0	1.5 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
SEL	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.0	0.0	±1.0

**10. Peak C sound level**

Number of cycle in test signal	Anticipated Value ( dB )	Measured Value, Lcpeak ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Continuous	133.0	133.0	0.0	±3.0
One	136.4	135.4	-1.0	±3.0

Number of cycle in test signal	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Continuous	133.0	133.0	0.0	±2.0
Positive half cycle	135.4	135.1	-0.3	±2.0
Negative half cycle	135.4	135.1	-0.3	±2.0

**เอกสารไม่ควบคุม**  
*T. Kethin.*



Cert. No. : ACL24055

Pages : 1 of 8

## Calibration Certificate

**Equipment :** SOUND LEVEL METER  
**Manufacturer :** RION  
**Model :** NL-42 / Microphone UC-52 / Preamplifier NH-24  
**Serial No.:** 00409175 / 185834 / 90621  
**ID No.:** UAE.EFM.014/2564

**Condition As Found :** GOOD

**Customer :** UNITED ANALYST AND ENGINEERING CONSULTANT (UAE)  
81 SOI UDOMSUK 41, SUKHUMVIT ROAD,  
BANGCHAK SUB-DISTRICT,  
PHRAKHANONG DISTRICT, BANGKOK 10260  
THAILAND.

**Location :** -

**Ambient Temperature :** ( 23.0  $\pm$  3 ) °C  
**Pressure :** ( 101.3  $\pm$  3 ) kPa  
**Relative Humidity :** ( 50.0  $\pm$  20 ) %

**Received Date :** 21 DECEMBER 2023  
**Calibration Date :** 18-19 JANUARY 2024  
**Date of Issue :** 22 JANUARY 2024

**Calibrated by :**

Nathakorn Pisutpaisan

**Approved by :**



( Thanakul Petchurai )

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

เอกสารไม่ควบคุม



# SITHIPORN ASSOCIATES CO., LTD.

## CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand  
Tel. +66 2433 8331 Email : calibration@sithiporn.com



Cert. No. : ACL24055  
Job No. : VC67AC0034  
Pages : 2 of 8

Calibration Procedure : CP-AC-01

### Calibration Method :

This equipment was calibrated by follow on IEC-61672-3 (2013) Standard for sound level meter (SLM).

The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.

For tests results of each items were made by observation of each Instruments display and also with SLM's display.

### Condition of this result of calibration :

#### 1. Reference Standard Instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
Waveform Generator	33210A	MY48017076	EF-0009-23	07-FEB-24
Waveform Generator	33511B	MY52302742	EF-0010-23	07-FEB-24
Digital Multimeter	33461A	MY53220104	EEL.BP 30/0266	13-FEB-24
Digital Multimeter	33461A	MY53220076	EEL.BP 29/0266	13-FEB-24
Digital Multimeter	34461A	MY60024273	EEL.BP 31/0266	14-FEB-24
Programmable Attenuator	MAT-1070	62100114	EF-0011-23	08-FEB-24
Condenser Microphone	4180	2977900	AA-1001-23	14-FEB-24
Measuring Amplifier	NA-42KAI	34560495	AA-3002-23	14-FEB-24

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is traceable to the international system of unit maintained at :

3.1 National Institute of Metrology (Thailand).

3.2 Thailand Institute of Scientific and Technological Research (TISTR).

เอกสารไม่ควบคุม  
7. Kethu

# SITHIPORN ASSOCIATES CO., LTD. CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand  
Tel. +66 2433 8331 Email : calibration@sithiporn.com

SITHIPORN  
associates



Cert. No. : ACL24055  
Job No. : VC67AC0034  
Pages : 3 of 8

## Summary of Measurement Result :

Parameter	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	0.2	N/A
2. Self-generated noise	0.2	N/A
3. Acoustical signal tests of frequency weightings		
125 Hz	0.3	0.6
1000 Hz	0.3	0.6
8000 Hz	0.3	0.7
4. Electrical signal tests of frequency weightings		
For 10 Hz to 4 kHz	0.3	0.6
For > 4 kHz to 10 kHz	0.3	0.7
For > 10 kHz to 20 kHz	-	1.0
5. Frequency and time weightings at 1 kHz	0.2	0.2
6. Long - term stability	0.1	0.1
7. Level linearity on the reference level range	0.2	0.3
8. Level linearity including the level range control	0.2	0.3
9. Tone burst response	0.2	0.3
10. Peak C sound level	0.2	0.35
11. Overload indication	0.2	0.25
12. High level stability	0.1	0.1

เอกสารไม่ควบคุม  
T. Kulkarni

**Cert. No. : ACL24055**

**Job No. : VC67AC0034**

**Pages : 4 of 8**

**Result of calibration :**

**1. Absolute sensitivity**

Reference Acoustic Signal ( dB )	Measured Value ( dB )	Deviation ( dB )	Acceptance Limit ( dB )
93.9 (93.98)	93.9	0.0	±0.3

**2. Self-generated noise**

**2.1 Normal test**

Measured Value ( dB )
16.4

**2.2 The microphone of the sound level meter was replaced by electrical signal input device.**

Frequency Weighting	Measured value ( dB )
A - weight	11.6
C - weight	17.8
Flat	23.8

**3. Acoustical signal tests of frequency weightings**

Meter free-field acoustic response at a level of 84 dB

Frequency ( Hz )	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
125	0.1	0.2	0.2	± 1.5
1000	0.0	0.0	0.0	± 1.0
8000	0.9	1.0	1.0	±5.0

**เอกสารไม่ควบคุม**  
*Y. Kela*

**Cert. No. : ACL24055**  
**Job No. : VC67AC0034**  
**Pages : 5 of 8**

#### 4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency ( Hz )	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	-0.1	0.0	0.0	±2.0
125	-0.1	0.1	0.0	±1.5
250	0.0	0.1	-0.1	±1.5
500	0.0	0.1	-0.1	±1.5
1000	-0.1	0.0	0.0	±1.0
2000	-0.1	0.1	0.0	±2.0
4000	-0.1	0.1	-0.1	±3.0
8000	0.0	0.1	0.0	±5.0

#### 5. Frequency and time weightings at 1 kHz

##### 5.1 Frequency weightings at 1 kHz

Frequency Weighting	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	94.0	94.0	0.0	± 0.2
C - weight	94.0	94.0	0.0	± 0.2
Flat	94.0	94.0	0.0	± 0.2

##### 5.2 Time weighting at 1 kHz

Frequency Weighting	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Fast	94.0	94.0	0.0	± 0.1
Slow	94.0	94.0	0.0	± 0.1
Leq	94.0	94.0	0.0	± 0.1

#### 6. Long - term stability

Frequency Weighting	SLM Display at initial ( dB )	SLM Display at final ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	94.0	94.1	0.1	± 0.2

**เอกสารไม่ควบคุม**  
*T. Kewin*



# SITHIPORN ASSOCIATES CO., LTD.

## CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand  
Tel. +66 2433 8331 Email : calibration@sithiporn.com

SITHIPORN  
associates



Cert. No. : ACL24055

Job No. : VC67AC0034

Pages : 6 of 8

### 7. Level linearity on the reference level range

Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
137.0	137.0	0.0	$\pm 1.1$
136.0	136.0	0.0	$\pm 1.1$
135.0	135.0	0.0	$\pm 1.1$
134.0	134.1	0.1	$\pm 1.1$
133.0	133.0	0.0	$\pm 1.1$
132.0	132.0	0.0	$\pm 1.1$
131.0	131.0	0.0	$\pm 1.1$
129.0	129.0	0.0	$\pm 1.1$
124.0	124.0	0.0	$\pm 1.1$
119.0	119.0	0.0	$\pm 1.1$
114.0	114.0	0.0	$\pm 1.1$
109.0	109.0	0.0	$\pm 1.1$
104.0	104.1	0.1	$\pm 1.1$
99.0	99.0	0.0	$\pm 1.1$
94.0	94.0	0.0	$\pm 1.1$
89.0	89.0	0.0	$\pm 1.1$
84.0	84.0	0.0	$\pm 1.1$
79.0	79.0	0.0	$\pm 1.1$
74.0	74.0	0.0	$\pm 1.1$
69.0	69.0	0.0	$\pm 1.1$
64.0	64.0	0.0	$\pm 1.1$
59.0	59.0	0.0	$\pm 1.1$
54.0	54.0	0.0	$\pm 1.1$
49.0	49.0	0.0	$\pm 1.1$
44.0	44.0	0.0	$\pm 1.1$
39.0	39.0	0.0	$\pm 1.1$
34.0	34.0	0.0	$\pm 1.1$
30.0	30.0	0.0	$\pm 1.1$
29.0	29.0	0.0	$\pm 1.1$
28.0	28.0	0.0	$\pm 1.1$
27.0	27.1	0.1	$\pm 1.1$
26.0	26.0	0.0	$\pm 1.1$
25.0	25.1	0.1	$\pm 1.1$

เอกสารไม่ควบคุม  
*E. Kelon*

# SITHIPORN ASSOCIATES CO., LTD. CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand  
Tel. +66 2433 8331 Email : calibration@sithiporn.com

SITHIPORN  
associates



Cert. No. : ACL24055

Job No. : VC67AC0034

Pages : 7 of 8

## 8. Level linearity including the level range control

Range	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Auto	94.0	94.0	0.0	±1.1

## 9. Tone burst response

Time Weighting	Tone burst duration, Tb ( ms )	Cycle	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	116.9	-0.1	1.0 ; -2.5
	200	800	134.0	134.0	0.0	±1.0
Slow	2	8	108.0	107.9	-0.1	1.5 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
SEL	0.25	1	99.0	98.8	-0.2	1.5 ; -5.0
	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.0	0.0	±1.0

## 10. Peak C sound level

Number of cycle in test signal	Anticipated Value ( dB )	Measured Value, Lcpeak ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Continuous	133.0	133.0	0.0	±3.0
One	136.4	136.3	-0.1	±3.0

Number of cycle in test signal	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Continuous	133.0	133.0	0.0	±2.0
Positive half cycle	135.4	135.1	-0.3	±2.0
Negative half cycle	135.4	135.1	-0.3	±2.0

เอกสารไม่ควบคุม  
T. Kewin

# SITHIPORN ASSOCIATES CO., LTD. CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand  
Tel. +66 2433 8331 Email : calibration@sithiporn.com

SITHIPORN  
associates



Cert. No. : ACL24055  
Job No. : VC67AC0034  
Pages : 8 of 8

## 11. Overload indication

Measured value ( dB )		Deviated Value ( dB )	Acceptance Limits ( dB )
Positive one-half cycle	Negative one-half cycle		
89.6	89.6	0.0	±1.5

## 12. High level stability

Frequency Weighting	SLM Display at initial ( dB )	SLM Display at final ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor  $k = 2$   
or any value following calculation, providing a level of confidence of approximately 95 %

————— End of Calibration Certificate —————

เอกสารไม่ควบคุม  
T. Kelen

# SITHIPORN ASSOCIATES CO., LTD. CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand  
Tel. +66 2433 8331 Email : calibration@sithiporn.com

SITHIPORN  
associates



Cert. No. : ACL24156  
Job No. : VC67AC0071  
Pages : 8 of 8

## 11. Overload indication

Measured value ( dB )		Deviated Value ( dB )	Acceptance Limits ( dB )
Positive one-half cycle	Negative one-half cycle		
89.7	89.5	-0.2	±1.5

## 12. High level stability

Frequency Weighting	SLM Display at initial ( dB )	SLM Display at final ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor  $k = 2$   
or any value following calculation, providing a level of confidence of approximately 95 %

End of Calibration Certificate

เอกสารไม่ควบคุม  
*E. Ketchu*



Cert. No. : ACL24059

Pages : 1 of 8

## Calibration Certificate

**Equipment :** SOUND LEVEL METER  
**Manufacturer :** RION  
**Model :** NL-42 / Microphone UC-52 / Preamplifier NH-24  
**Serial No.:** 00709651 / 188529 / 00801  
**ID No.:** UAE.EFM.019/2564

**Condition As Found :** GOOD

**Customer :** UNITED ANALYST AND ENGINEERING CONSULTANT (UAE)  
81 SOI UDOMSUK 41, SUKHUMVIT ROAD,  
BANGCHAK SUB-DISTRICT,  
PHRAKHANONG DISTRICT, BANGKOK 10260  
THAILAND.

**Location :** -

**Ambient Temperature :** ( 23.0  $\pm$  3 ) °C  
**Pressure :** ( 101.3  $\pm$  3 ) kPa  
**Relative Humidity :** ( 50.0  $\pm$  20 ) %

**Received Date :** 21 DECEMBER 2023  
**Calibration Date :** 18-19 JANUARY 2024  
**Date of Issue :** 22 JANUARY 2024

**Calibrated by :**

Nathakorn Pisutpaisan

**Approved by :**

*T. Petchurai*  
( Thanakul Petchurai )

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

เอกสารไม่ควบคุม

# SITHIPORN ASSOCIATES CO., LTD.

## CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand  
Tel. +66 2433 8331 Email : calibration@sithiporn.com



Cert. No. : ACL24059  
Job No. : VC67AC0034  
Pages : 2 of 8

Calibration Procedure : CP-AC-01

### Calibration Method :

This equipment was calibrated by follow on IEC-61672-3 (2013) Standard for sound level meter (SLM).

The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.

For tests results of each items were made by observation of each Instruments display and also with SLM's display.

### Condition of this result of calibration :

#### 1. Reference Standard Instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
Waveform Generator	33210A	MY48017076	EF-0009-23	07-FEB-24
Waveform Generator	33511B	MY52302742	EF-0010-23	07-FEB-24
Digital Multimeter	33461A	MY53220104	EEL.BP 30/0266	13-FEB-24
Digital Multimeter	33461A	MY53220076	EEL.BP 29/0266	13-FEB-24
Digital Multimeter	34461A	MY60024273	EEL.BP 31/0266	14-FEB-24
Programmable Attenuator	MAT-1070	62100114	EF-0011-23	08-FEB-24
Condenser Microphone	4180	2977900	AA-1001-23	14-FEB-24
Measuring Amplifier	NA-42KAI	34560495	AA-3002-23	14-FEB-24

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is traceable to the international system of unit maintained at :

3.1 National Institute of Metrology (Thailand).

3.2 Thailand Institute of Scientific and Technological Research (TISTR).

เอกสารไม่ควบคุม  
7. Kela

# SITHIPORN ASSOCIATES CO., LTD. CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand  
Tel. +66 2433 8331 Email : calibration@sithiporn.com

SITHIPORN  
associates



Cert. No. : ACL24059  
Job No. : VC67AC0034  
Pages : 3 of 8

## Summary of Measurement Result :

Parameter	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	0.2	N/A
2. Self-generated noise	0.2	N/A
3. Acoustical signal tests of frequency weightings		
125 Hz	0.3	0.6
1000 Hz	0.3	0.6
8000 Hz	0.3	0.7
4. Electrical signal tests of frequency weightings		
For 10 Hz to 4 kHz	0.3	0.6
For > 4 kHz to 10 kHz	0.3	0.7
For > 10 kHz to 20 kHz	-	1.0
5. Frequency and time weightings at 1 kHz	0.2	0.2
6. Long - term stability	0.1	0.1
7. Level linearity on the reference level range	0.2	0.3
8. Level linearity including the level range control	0.2	0.3
9. Tone burst response	0.2	0.3
10. Peak C sound level	0.2	0.35
11. Overload indication	0.2	0.25
12. High level stability	0.1	0.1

เอกสารไม่ควบคุม  
*[Signature]*

# SITHIPORN ASSOCIATES CO., LTD. CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand  
Tel. +66 2433 8331 Email : calibration@sithiporn.com

SITHIPORN  
associates



Cert. No. : ACL24059

Job No. : VC67AC0034

Pages : 4 of 8

## Result of calibration :

### 1. Absolute sensitivity

Reference Acoustic Signal ( dB )	Measured Value ( dB )	Deviation ( dB )	Acceptance Limit ( dB )
93.9 (93.98)	93.9	0.0	±0.3

### 2. Self-generated noise

#### 2.1 Normal test

Measured Value ( dB )
14.6

#### 2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Measured value ( dB )
A - weight	10.8
C - weight	17.2
Flat	23.1

### 3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency ( Hz )	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
125	0.2	0.3	0.3	± 1.5
1000	0.1	0.1	0.1	± 1.0
8000	0.7	0.8	0.8	±5.0

เอกสารไม่ควบคุม  
T. Ketch



**Cert. No. : ACL24059**  
**Job No. : VC67AC0034**  
**Pages : 5 of 8**

#### 4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency ( Hz )	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	-0.1	-0.1	-0.1	±2.0
125	0.0	0.0	0.0	±1.5
250	0.0	0.0	-0.1	±1.5
500	0.0	0.0	-0.1	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.0	0.0	±2.0
4000	0.0	0.0	0.0	±3.0
8000	0.0	0.0	0.0	±5.0

#### 5. Frequency and time weightings at 1 kHz

##### 5.1 Frequency weightings at 1 kHz

Frequency Weighting	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	94.0	94.0	0.0	± 0.2
C - weight	94.0	94.0	0.0	± 0.2
Flat	94.0	94.0	0.0	± 0.2

##### 5.2 Time weighting at 1 kHz

Frequency Weighting	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Fast	94.0	94.0	0.0	± 0.1
Slow	94.0	94.0	0.0	± 0.1
Leq	94.0	94.0	0.0	± 0.1

#### 6. Long - term stability

Frequency Weighting	SLM Display at initial ( dB )	SLM Display at final ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	94.0	94.0	0.0	± 0.2

เอกสารไม่ควบคุม

T. Kelen

# SITHIPORN ASSOCIATES CO., LTD.

## CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand  
Tel. +66 2433 8331 Email : calibration@sithiporn.com

SITHIPORN  
associates



Cert. No. : ACL24059

Job No. : VC67AC0034

Pages : 6 of 8

### 7. Level linearity on the reference level range

Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
137.0	137.1	0.1	$\pm 1.1$
136.0	136.1	0.1	$\pm 1.1$
135.0	135.1	0.1	$\pm 1.1$
134.0	134.1	0.1	$\pm 1.1$
133.0	133.0	0.0	$\pm 1.1$
132.0	132.0	0.0	$\pm 1.1$
131.0	131.0	0.0	$\pm 1.1$
129.0	129.1	0.1	$\pm 1.1$
124.0	124.0	0.0	$\pm 1.1$
119.0	119.1	0.1	$\pm 1.1$
114.0	114.1	0.1	$\pm 1.1$
109.0	109.1	0.1	$\pm 1.1$
104.0	104.1	0.1	$\pm 1.1$
99.0	99.1	0.1	$\pm 1.1$
94.0	94.0	0.0	$\pm 1.1$
89.0	89.0	0.0	$\pm 1.1$
84.0	84.0	0.0	$\pm 1.1$
79.0	79.0	0.0	$\pm 1.1$
74.0	74.0	0.0	$\pm 1.1$
69.0	69.0	0.0	$\pm 1.1$
64.0	64.0	0.0	$\pm 1.1$
59.0	59.0	0.0	$\pm 1.1$
54.0	54.0	0.0	$\pm 1.1$
49.0	49.0	0.0	$\pm 1.1$
44.0	44.0	0.0	$\pm 1.1$
39.0	39.0	0.0	$\pm 1.1$
34.0	34.0	0.0	$\pm 1.1$
30.0	30.0	0.0	$\pm 1.1$
29.0	29.1	0.1	$\pm 1.1$
28.0	28.0	0.0	$\pm 1.1$
27.0	27.0	0.0	$\pm 1.1$
26.0	26.1	0.1	$\pm 1.1$
25.0	25.2	0.2	$\pm 1.1$

เอกสารไม่ควบคุม  
7. Relate -

# SITHIPORN ASSOCIATES CO., LTD.

## CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand  
Tel. +66 2433 8331 Email : calibration@sithiporn.com

SITHIPORN  
associates



Cert. No. : ACL24059

Job No. : VC67AC0034

Pages : 7 of 8

### 8. Level linearity including the level range control

Range	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Auto	94.0	94.0	0.0	±1.1

### 9. Tone burst response

Time Weighting	Tone burst duration, Tb ( ms )	Cycle	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.0	0.0	±1.0
Slow	2	8	108.0	108.0	0.0	1.5 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
SEL	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.0	0.0	±1.0

### 10. Peak C sound level

Number of cycle in test signal	Anticipated Value ( dB )	Measured Value, Lcpeak ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Continuous	133.0	133.0	0.0	±3.0
One	136.4	136.1	-0.3	±3.0

Number of cycle in test signal	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Continuous	133.0	133.0	0.0	±2.0
Positive half cycle	135.4	135.1	-0.3	±2.0
Negative half cycle	135.4	135.1	-0.3	±2.0

เอกสารไม่ควบคุม  
T. Kewin

# SITHIPORN ASSOCIATES CO., LTD.

## CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand  
Tel, +66 2433 8331 Email : calibration@sithiporn.com

SITHIPORN  
associates



Cert. No. : ACL24059

Job No. : VC67AC0034

Pages : 8 of 8

### 11. Overload indication

Measured value ( dB )		Deviated Value ( dB )	Acceptance Limits ( dB )
Positive one-half cycle	Negative one-half cycle		
89.6	89.5	-0.1	±1.5

### 12. High level stability

Frequency Weighting	SLM Display at initial ( dB )	SLM Display at final ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor  $k = 2$   
or any value following calculation, providing a level of confidence of approximately 95 %

————— End of Calibration Certificate —————

เอกสารไม่ควบคุม  
Y. K. K.



## Certificate of Calibration

### Customer

Name : UNITED ANALYST AND ENGINEERING  
CONSULTANT CO.,LTD.

Certificate No : 24-ACT-065

Request No : Req-2024-1022

Address : 81 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Prakanong,  
Bangkok 10260

### Unit Under Calibration Details

Measurement item : Acoustic Calibrator

Class : 1

Manufacturer : 01dB

Range : 94 dB / 1000 Hz

Model : CAL31

Instrument Status : Used

Serial Number : 82795

ID : UAE.EFM.113/2560

### Calibration Environment and Details

Temperature : ( 23 ±2 °C )

Humidity : ( 50 ± 20 %RH )

Barometric Pressure : ( 1013 ±10.0 hPa )

Received Date : 8 May 2024

Calibration Date : 17 May 2024

Location of Calibration : LAB 1 Acoustic

Calibration Procedure : In-house method CP-ACT-02 based on IEC 60942:2017 Electroacoustics - Sound calibrators

Reference Standard	Model	Serial Number	Traceable	Due Calibration
Sound Calibrator	SV 35A	58079	EEI	31 May 2024
THD Multimeter	2015	1047765	NIMT	16 January 2025

**Traceability** : This certificate provides traceability of measurement to recognized national standard, and to the realization of the international System of Units (SI).

### Note

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor k=2, providing a level of confidence approximately 95 %.

Calibrated By :



Mr. Noppadon Luangart  
Service Calibration Engineer

Approved By :



Mr. Pacit Mathavorn  
Calibration Engineer Supervisor

Issue Date : 17 May 2024

Certificate No : 24-ACT-065

Request No : Req-2024-1022

**Sound pressure level**

**Calibration Results : Without Adjustment**

Calibration Range (dB)	Without Adjustment (dB)		Adjustment (dB)		Uncertainty ( ± dB)	Acceptance limit Class 1 ( ± dB)
	Measured	Deviated value	Measured	Deviated value		
94 dB / 1000 Hz	94.17	0.17	-	-	0.13	0.25

**Frequency of Sound pressure level**

Calibration Range (Hz)	Without Adjustment		Adjustment		Uncertainty ( ± %)	Acceptance limit Class 1 ( ± %)
	Measured (Hz)	Deviated value	Measured (Hz)	Deviated value		
94 dB / 1000 Hz	1000.00	0.00	-	-	0.01	0.70

**Total Harmonic Distortion plus Noise of Sound pressure level (THD+N %)**

Calibration Range (Hz)	Without Adjustment	Adjustment	Uncertainty ( ± %)	Acceptance limit Class 1 ( ± %)
	Measured (%)	Measured (%)		
94 dB / 1000 Hz	0.09	-	0.40	2.5

**Note :**

Function	Maximum-permitted Uncertainty of measurement
Sound pressure level	0.15 dB
Frequency	0.20%
Total distortion+noise	0.50%

- Acceptance limit was IEC60942:2017 Class 1

- The calibration results exclude the calibrator pressure correction

- The calibration results exclude the microphone volume correction

**End of Calibration**

**Cert. No. : ACL24155**

**Pages : 1 of 8**

## Calibration Certificate

**Equipment :** SOUND LEVEL METER  
**Manufacturer :** RION  
**Model :** NL-42 / Microphone UC-52 / Preamplifier NH-24  
**Serial No.:** 00709656 / 189028 / 01207  
**ID No.:** UAE.EFM.021/2564

**Condition As Found :** GOOD

**Customer :** UNITED ANALYST AND ENGINEERING CONSULTANT (UAE)  
81 SOI UDOMSUK 41, SUKHUMVIT ROAD,  
BANGCHAK SUB-DISTRICT,  
PHRAKHANONG DISTRICT, BANGKOK 10260  
THAILAND.

**Location :** -  
**Ambient Temperature :** ( 23.0  $\pm$  3 ) °C  
**Pressure :** ( 101.3  $\pm$  3 ) kPa  
**Relative Humidity :** ( 50.0  $\pm$  20 ) %

**Received Date :** 10 MAY 2024  
**Calibration Date :** 30 - 31 MAY 2024  
**Date of Issue :** 04 JUNE 2024

**Calibrated by :** Nathakorn Pisutpaisan

**Approved by :**

  
( Thanakul Petchurai )

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

**เอกสารไม่ควบคุม**

# SITHIPORN ASSOCIATES CO., LTD.

## CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand  
Tel. +66 2433 8331 Email : calibration@sithiporn.com

SITHIPORN  
associates



Cert. No. : ACL24155  
Job No. : VC67AC0071  
Pages : 2 of 8

Calibration Procedure : CP-AC-01

### Calibration Method :

This equipment was calibrated by follow on IEC-61672-3 (2013) Standard for sound level meter (SLM).

The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.

For tests results of each items were made by observation of each Instruments display and also with SLM's display.

### Condition of this result of calibration :

#### 1. Reference Standard Instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
Waveform Generator	33210A	MY48017076	EF-0009-24	05-FEB-25
Waveform Generator	33511B	MY52302742	EF-0007-24	05-FEB-25
Digital Multimeter	33461A	MY53220104	EEL.BP 21/0267	13-FEB-25
Digital Multimeter	33461A	MY53220076	EEL.BP 20/0267	15-FEB-25
Digital Multimeter	34461A	MY60024273	EEL.BP 22/0267	15-FEB-25
Programmable Attenuator	MAT-1070	62100114	EF-0008-24	05-FEB-25
Condenser Microphone	4180	2977900	AA-1001-24	12-FEB-25
Measuring Amplifier	NA-42KAI	34560495	AA-3001-24	05-FEB-25

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is traceable to the international system of unit maintained at :

3.1 National Institute of Metrology (Thailand).

3.2 Thailand Institute of Scientific and Technological Research (TISTR).

เอกสารไม่ควบคุม  
T. Ketchu



# SITHIPORN ASSOCIATES CO., LTD.

## CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand  
Tel. +66 2433 8331 Email : calibration@sithiporn.com

SITHIPORN  
associates



Cert. No. : ACL24155

Job No. : VC67AC0071

Pages : 3 of 8

### Summary of Measurement Result :

Parameter	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	0.2	N/A
2. Self-generated noise	0.2	N/A
3. Acoustical signal tests of frequency weightings		
125 Hz	0.3	0.6
1000 Hz	0.3	0.6
8000 Hz	0.3	0.7
4. Electrical signal tests of frequency weightings		
For 10 Hz to 4 kHz	0.3	0.6
For > 4 kHz to 10 kHz	0.3	0.7
For > 10 kHz to 20 kHz	-	1.0
5. Frequency and time weightings at 1 kHz	0.2	0.2
6. Long - term stability	0.1	0.1
7. Level linearity on the reference level range	0.2	0.3
8. Level linearity including the level range control	0.2	0.3
9. Tone burst response	0.2	0.3
10. Peak C sound level	0.2	0.35
11. Overload indication	0.2	0.25
12. High level stability	0.1	0.1

เอกสารไม่ควบคุม  
*T. Rekh*

**Cert. No. : ACL24155**

**Job No. : VC67AC0071**

**Pages : 4 of 8**

**Result of calibration :**

**1. Absolute sensitivity**

Reference Acoustic Signal ( dB )	Measured Value ( dB )	Deviation ( dB )	Acceptance Limit ( dB )
93.9 (93.94)	93.9	0.0	±0.3

**2. Self-generated noise**

**2.1 Normal test**

Measured Value ( dB )
14.8

**2.2** The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Measured value ( dB )
A - weight	13.4
C - weight	19.7
Flat	25.1

**3. Acoustical signal tests of frequency weightings**

Meter free-field acoustic response at a level of 84 dB

Frequency ( Hz )	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
125	0.0	0.0	0.0	± 1.5
1000	-0.1	-0.1	-0.1	± 1.0
8000	1.2	1.3	1.2	±5.0

**เอกสารไม่ควบคุม**  
*T. Kewin*

**Cert. No. : ACL24155**

**Job No. : VC67AC0071**

**Pages : 5 of 8**

#### 4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency ( Hz )	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	-0.1	-0.1	-0.1	±2.0
125	0.0	0.0	0.0	±1.5
250	0.0	0.0	0.0	±1.5
500	0.0	0.0	0.0	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.0	0.0	±2.0
4000	0.0	0.0	0.0	±3.0
8000	0.0	0.1	0.1	±5.0

#### 5. Frequency and time weightings at 1 kHz

##### 5.1 Frequency weightings at 1 kHz

Frequency Weighting	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	94.0	94.0	0.0	± 0.2
C - weight	94.0	94.0	0.0	± 0.2
Flat	94.0	94.0	0.0	± 0.2

##### 5.2 Time weighting at 1 kHz

Frequency Weighting	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Fast	94.0	94.0	0.0	± 0.1
Slow	94.0	94.0	0.0	± 0.1
Leq	94.0	94.0	0.0	± 0.1

#### 6. Long - term stability

Frequency Weighting	SLM Display at initial ( dB )	SLM Display at final ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	94.0	94.0	0.0	

**เอกสารไม่ควบคุม**

*T. K.*

# SITHIPORN ASSOCIATES CO., LTD.

## CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand  
Tel. +66 2433 8331 Email : calibration@sithiporn.com

SITHIPORN  
associates



Cert. No. : ACL24155

Job No. : VC67AC0071

Pages : 6 of 8

### 7. Level linearity on the reference level range

Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
137.0	137.0	0.0	± 1.1
136.0	136.0	0.0	± 1.1
135.0	135.0	0.0	± 1.1
134.0	134.0	0.0	± 1.1
133.0	133.0	0.0	± 1.1
132.0	132.0	0.0	± 1.1
131.0	131.0	0.0	± 1.1
129.0	129.0	0.0	± 1.1
124.0	124.0	0.0	± 1.1
119.0	119.0	0.0	± 1.1
114.0	114.0	0.0	± 1.1
109.0	109.0	0.0	± 1.1
104.0	104.0	0.0	± 1.1
99.0	99.0	0.0	± 1.1
94.0	94.0	0.0	± 1.1
89.0	89.0	0.0	± 1.1
84.0	84.0	0.0	± 1.1
79.0	79.0	0.0	± 1.1
74.0	74.0	0.0	± 1.1
69.0	69.0	0.0	± 1.1
64.0	64.0	0.0	± 1.1
59.0	59.0	0.0	± 1.1
54.0	54.0	0.0	± 1.1
49.0	49.0	0.0	± 1.1
44.0	44.0	0.0	± 1.1
39.0	39.0	0.0	± 1.1
34.0	34.0	0.0	± 1.1
30.0	30.1	0.1	± 1.1
29.0	29.1	0.1	± 1.1
28.0	28.1	0.1	± 1.1
27.0	27.2	0.2	± 1.1
26.0	26.3	0.3	± 1.1
25.0	25.3	0.3	± 1.1

เอกสารไม่ควบคุม

7. Rev. 1



**Cert. No. : ACL24155**  
**Job No. : VC67AC0071**  
**Pages : 7 of 8**

**8. Level linearity including the level range control**

Range	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Auto	94.0	94.0	0.0	±1.1

**9. Tone burst response**

Time Weighting	Tone burst duration, Tb ( ms )	Cycle	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.0	0.0	±1.0
Slow	2	8	108.0	108.0	0.0	1.5 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
SEL	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.0	0.0	±1.0

**10. Peak C sound level**

Number of cycle in test signal	Anticipated Value ( dB )	Measured Value, Lcpeak ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Continuous	133.0	133.0	0.0	±3.0
One	136.4	136.2	-0.2	±3.0

Number of cycle in test signal	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Continuous	133.0	133.0	0.0	±2.0
Positive half cycle	135.4	135.2	-0.2	±2.0
Negative half cycle	135.4	135.2	-0.2	±2.0

**เอกสารไม่ควบคุม**  


# SITHIPORN ASSOCIATES CO., LTD. CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand  
Tel. +66 2433 8331 Email : calibration@sithiporn.com

SITHIPORN  
associates



Cert. No. : ACL24155  
Job No. : VC67AC0071  
Pages : 8 of 8

## 11. Overload indication

Measured value ( dB )		Deviated Value ( dB )	Acceptance Limits ( dB )
Positive one-half cycle	Negative one-half cycle		
89.6	89.5	-0.1	±1.5

## 12. High level stability

Frequency Weighting	SLM Display at initial ( dB )	SLM Display at final ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor  $k = 2$   
or any value following calculation, providing a level of confidence of approximately 95 %

————— End of Calibration Certificate —————

เอกสารไม่ควบคุม  
*T. Petch.*

Cert. No. : ACL24098

Pages : 1 of 8

## Calibration Certificate

**Equipment :** SOUND LEVEL METER  
**Manufacturer :** RION  
**Model :** NL-42 / Microphone UC-52 / Preamplifier NH-24  
**Serial No.:** 00408981 / 186171 / 90426  
**ID No.:** UAE.EFM.008/2564

**Condition As Found :** GOOD

**Customer :** UNITED ANALYST AND ENGINEERING CONSULTANT (UAE)  
81 SOI UDOMSUK 41, SUKHUMVIT ROAD,  
BANGCHAK SUB-DISTRICT,  
PHRAKHANONG DISTRICT, BANGKOK 10260  
THAILAND.

**Location :** -  
**Ambient Temperature :** ( 23.0  $\pm$  3 ) °C  
**Pressure :** ( 101.3  $\pm$  3 ) kPa  
**Relative Humidity :** ( 50.0  $\pm$  20 ) %

**Received Date :** 18 JANUARY 2024  
**Calibration Date :** 29-30 JANUARY 2024  
**Date of Issue :** 02 FEBRUARY 2024

**Calibrated by :** Nathakorn Pisutpaisan

**Approved by :**

  
( Thanakul Petchurai )

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

เอกสารไม่ควบคุม

# SITHIPORN ASSOCIATES CO., LTD.

## CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand  
Tel. +66 2433 8331 Email : calibration@sithiporn.com



Cert. No. : ACL24098  
Job No. : VC67AC0057  
Pages : 2 of 8

Calibration Procedure : CP-AC-01

### Calibration Method :

This equipment was calibrated by follow on IEC-61672-3 (2013) Standard for sound level meter (SLM).

The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.

For tests results of each items were made by observation of each Instruments display and also with SLM's display.

### Condition of this result of calibration :

#### 1. Reference Standard Instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
Waveform Generator	33210A	MY48017076	EF-0009-23	07-FEB-24
Waveform Generator	33511B	MY52302742	EF-0010-23	07-FEB-24
Digital Multimeter	33461A	MY53220104	EEL.BP 30/0266	13-FEB-24
Digital Multimeter	33461A	MY53220076	EEL.BP 29/0266	13-FEB-24
Digital Multimeter	34461A	MY60024273	EEL.BP 31/0266	14-FEB-24
Programmable Attenuator	MAT-1070	62100114	EF-0011-23	08-FEB-24
Condenser Microphone	4180	2977900	AA-1001-23	14-FEB-24
Measuring Amplifier	NA-42KAI	34560495	AA-3002-23	14-FEB-24

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is traceable to the international system of unit maintained at :

3.1 National Institute of Metrology (Thailand).

3.2 Thailand Institute of Scientific and Technological Research (TISTR).

เอกสารไม่ควบคุม  
*[Signature]*



# SITHIPORN ASSOCIATES CO., LTD.

## CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand  
Tel. +66 2433 8331 Email : calibration@sithiporn.com

SITHIPORN  
associates



Cert. No. : ACL24098  
Job No. : VC67AC0057  
Pages : 3 of 8

### Summary of Measurement Result :

Parameter	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	0.2	N/A
2. Self-generated noise	0.2	N/A
3. Acoustical signal tests of frequency weightings		
125 Hz	0.3	0.6
1000 Hz	0.3	0.6
8000 Hz	0.3	0.7
4. Electrical signal tests of frequency weightings		
For 10 Hz to 4 kHz	0.3	0.6
For > 4 kHz to 10 kHz	0.3	0.7
For > 10 kHz to 20 kHz	-	1.0
5. Frequency and time weightings at 1 kHz	0.2	0.2
6. Long - term stability	0.1	0.1
7. Level linearity on the reference level range	0.2	0.3
8. Level linearity including the level range control	0.2	0.3
9. Tone burst response	0.2	0.3
10. Peak C sound level	0.2	0.35
11. Overload indication	0.2	0.25
12. High level stability	0.1	0.1

เอกสารไม่ควบคุม  
T. Kech

# SITHIPORN ASSOCIATES CO., LTD.

## CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand  
Tel. +66 2433 8331 Email : calibration@sithiporn.com

SITHIPORN  
associates



Cert. No. : ACL24098

Job No. : VC67AC0057

Pages : 4 of 8

### Result of calibration :

#### 1. Absolute sensitivity

Reference Acoustic Signal ( dB )	Measured Value ( dB )	Deviation ( dB )	Acceptance Limit ( dB )
93.9 (93.98)	93.9	0.0	±0.3

#### 2. Self-generated noise

##### 2.1 Normal test

Measured Value ( dB )
14.6

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Measured value ( dB )
A - weight	10.8
C - weight	16.8
Flat	23.0

#### 3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency ( Hz )	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
125	0.5	0.5	0.5	± 1.5
1000	0.0	0.0	0.0	± 1.0
8000	1.0	1.0	1.0	±5.0

เอกสารไม่ควบคุม  
T. Kewin

**Cert. No. : ACL24098**  
**Job No. : VC67AC0057**  
**Pages : 5 of 8**

#### 4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency ( Hz )	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	0.0	-0.2	-0.1	±2.0
125	-0.1	0.0	-0.1	±1.5
250	0.0	-0.1	-0.1	±1.5
500	0.0	0.0	-0.1	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.0	0.0	±2.0
4000	0.0	0.0	0.0	±3.0
8000	0.0	0.0	0.0	±5.0

#### 5. Frequency and time weightings at 1 kHz

##### 5.1 Frequency weightings at 1 kHz

Frequency Weighting	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	94.0	94.0	0.0	± 0.2
C - weight	94.0	94.0	0.0	± 0.2
Flat	94.0	94.0	0.0	± 0.2

##### 5.2 Time weighting at 1 kHz

Frequency Weighting	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Fast	94.0	94.0	0.0	± 0.1
Slow	94.0	94.0	0.0	± 0.1
Leq	94.0	94.0	0.0	± 0.1

#### 6. Long - term stability

Frequency Weighting	SLM Display at initial ( dB )	SLM Display at final ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	94.0	94.0	0.0	± 0.3

เอกสารไม่ควบคุม  
 T. Kelen

# SITHIPORN ASSOCIATES CO., LTD.

## CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand  
Tel. +66 2433 8331 Email : calibration@sithiporn.com

SITHIPORN  
associates



Cert. No. : ACL24098

Job No. : VC67AC0057

Pages : 6 of 8

### 7. Level linearity on the reference level range

Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
137.0	137.1	0.1	$\pm 1.1$
136.0	136.1	0.1	$\pm 1.1$
135.0	135.1	0.1	$\pm 1.1$
134.0	134.1	0.1	$\pm 1.1$
133.0	133.0	0.0	$\pm 1.1$
132.0	132.0	0.0	$\pm 1.1$
131.0	131.0	0.0	$\pm 1.1$
129.0	129.1	0.1	$\pm 1.1$
124.0	124.0	0.0	$\pm 1.1$
119.0	119.1	0.1	$\pm 1.1$
114.0	114.1	0.1	$\pm 1.1$
109.0	109.1	0.1	$\pm 1.1$
104.0	104.1	0.1	$\pm 1.1$
99.0	99.1	0.1	$\pm 1.1$
94.0	94.0	0.0	$\pm 1.1$
89.0	89.0	0.0	$\pm 1.1$
84.0	84.0	0.0	$\pm 1.1$
79.0	79.0	0.0	$\pm 1.1$
74.0	74.0	0.0	$\pm 1.1$
69.0	69.0	0.0	$\pm 1.1$
64.0	64.0	0.0	$\pm 1.1$
59.0	59.0	0.0	$\pm 1.1$
54.0	54.0	0.0	$\pm 1.1$
49.0	49.0	0.0	$\pm 1.1$
44.0	44.0	0.0	$\pm 1.1$
39.0	39.0	0.0	$\pm 1.1$
34.0	34.0	0.0	$\pm 1.1$
30.0	29.9	-0.1	$\pm 1.1$
29.0	28.9	-0.1	$\pm 1.1$
28.0	27.9	-0.1	$\pm 1.1$
27.0	26.9	-0.1	$\pm 1.1$
26.0	25.9	-0.1	$\pm 1.1$
25.0	24.9	-0.1	$\pm 1.1$

เอกสารไม่ควบคุม  
7. Recheck -



**Cert. No. : ACL24098**  
**Job No. : VC67AC0057**  
**Pages : 7 of 8**

**8. Level linearity including the level range control**

Range	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Auto	94.0	94.0	0.0	±1.1

**9. Tone burst response**

Time Weighting	Tone burst duration, Tb ( ms )	Cycle	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.0	0.0	±1.0
Slow	2	8	108.0	108.0	0.0	1.5 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
SEL	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.0	0.0	±1.0

**10. Peak C sound level**

Number of cycle in test signal	Anticipated Value ( dB )	Measured Value, Lcpeak ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Continuous	133.0	133.0	0.0	±3.0
One	136.4	135.9	-0.5	±3.0

Number of cycle in test signal	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Continuous	133.0	133.0	0.0	±2.0
Positive half cycle	135.4	135.1	-0.3	±2.0
Negative half cycle	135.4	135.1	-0.3	±2.0

**เอกสารไม่ควบคุม**  
*7. K. K.*

# SITHIPORN ASSOCIATES CO., LTD. CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand  
Tel. +66 2433 8331 Email : calibration@sithiporn.com

SITHIPORN  
associates



Cert. No. : ACL24098  
Job No. : VC67AC0057  
Pages : 8 of 8

## 11. Overload indication

Measured value ( dB )		Deviated Value ( dB )	Acceptance Limits ( dB )
Positive one-half cycle	Negative one-half cycle		
89.5	89.5	0.0	±1.5

## 12. High level stability

Frequency Weighting	SLM Display at initial ( dB )	SLM Display at final ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor  $k = 2$   
or any value following calculation, providing a level of confidence of approximately 95 %

————— End of Calibration Certificate —————

เอกสารไม่ควบคุม  
*T. Ketch.*

Cert. No. : ACL24159

Pages : 1 of 8

## Calibration Certificate

**Equipment :** SOUND LEVEL METER  
**Manufacturer :** RION  
**Model :** NL-62 / Microphone UC-59L / Preamplifier NH-26  
**Serial No.:** 00511774 / 02238 / 11972  
**ID No.:** UAE.EFM.090/2565

**Condition As Found :** GOOD

**Customer :** UNITED ANALYST AND ENGINEERING CONSULTANT (UAE)  
81 SOI UDOMSUK 41, SUKHUMVIT ROAD,  
BANGCHAK SUB-DISTRICT,  
PHRAKHANONG DISTRICT, BANGKOK 10260  
THAILAND.

**Location :** -

**Ambient Temperature :** ( 23.0  $\pm$  3 ) °C  
**Pressure :** ( 101.3  $\pm$  3 ) kPa  
**Relative Humidity :** ( 50.0  $\pm$  20 ) %

**Received Date :** 10 MAY 2024  
**Calibration Date :** 04 - 05 JUNE 2024  
**Date of Issue :** 06 JUNE 2024

**Calibrated by :**

Nathakorn Pisutpaisan

**Approved by :**

  
( Thanakul Petchurai )

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

เอกสารไม่ควบคุม

# SITHIPORN ASSOCIATES CO., LTD. CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbunru, Bangplud, Bangkok, 10700 Thailand  
Tel. +66 2433 8331 Email : calibration@sithiporn.com

SITHIPORN  
associates



Cert. No. : ACL24159  
Job No. : VC67AC0071  
Pages : 2 of 8

Calibration Procedure : CP-AC-01

## Calibration Method :

This equipment was calibrated by follow on IEC-61672-3 (2013) Standard for sound level meter (SLM).

The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.

For tests results of each items were made by observation of each Instruments display and also with SLM's display.

## Condition of this result of calibration :

### 1. Reference Standard Instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
Waveform Generator	33210A	MY48017076	EF-0009-24	05-FEB-25
Waveform Generator	33511B	MY52302742	EF-0007-24	05-FEB-25
Digital Multimeter	33461A	MY53220104	EEL.BP 21/0267	13-FEB-25
Digital Multimeter	33461A	MY53220076	EEL.BP 20/0267	15-FEB-25
Digital Multimeter	34461A	MY60024273	EEL.BP 22/0267	15-FEB-25
Programmable Attenuator	MAT-1070	62100114	EF-0008-24	05-FEB-25
Condenser Microphone	4180	2977900	AA-1001-24	12-FEB-25
Measuring Amplifier	NA-42KAI	34560495	AA-3001-24	05-FEB-25

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is traceable to the international system of unit maintained at :

3.1 National Institute of Metrology (Thailand).

3.2 Thailand Institute of Scientific and Technological Research (TISTR).

เอกสารไม่ควบคุม  
*[Signature]*



# SITHIPORN ASSOCIATES CO., LTD. CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand  
Tel. +66 2433 8331 Email : calibration@sithiporn.com

SITHIPORN  
associates



Cert. No. : ACL24159  
Job No. : VC67AC0071  
Pages : 3 of 8

## Summary of Measurement Result :

Parameter	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	0.2	N/A
2. Self-generated noise	0.3	N/A
3. Acoustical signal tests of frequency weightings		
125 Hz	0.3	0.6
1000 Hz	0.3	0.6
8000 Hz	0.3	0.7
4. Electrical signal tests of frequency weightings		
For 10 Hz to 4 kHz	0.3	0.6
For > 4 kHz to 10 kHz	0.3	0.7
For > 10 kHz to 20 kHz	0.3	1.0
5. Frequency and time weightings at 1 kHz	0.2	0.2
6. Long - term stability	0.1	0.1
7. Level linearity on the reference level range	0.2	0.3
8. Level linearity including the level range control	0.2	0.3
9. Tone burst response	0.2	0.3
10. Peak C sound level	0.2	0.35
11. Overload indication	0.2	0.25
12. High level stability	0.1	0.1

เอกสารไม่ควบคุม  
*[Signature]*

**Cert. No. : ACL24159**

**Job No. : VC67AC0071**

**Pages : 4 of 8**

**Result of calibration :**

**1. Absolute sensitivity**

Reference Acoustic Signal ( dB )	Measured Value ( dB )	Deviation ( dB )	Acceptance Limit ( dB )
93.9 (93.94)	94.0	0.0	±0.3

**2. Self-generated noise**

**2.1 Normal test**

Measured Value ( dB )
15.6

**2.2 The microphone of the sound level meter was replaced by electrical signal input device.**

Frequency Weighting	Measured value ( dB )
A - weight	11.6
C - weight	16.8
Flat	24.9

**3. Acoustical signal tests of frequency weightings**

Meter free-field acoustic response at a level of 84 dB

Frequency ( Hz )	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
125	0.2	0.2	0.2	± 1.0
1000	0.0	0.0	0.0	± 0.7
8000	-0.2	-0.2	-0.2	+ 1.5, - 2.5

**เอกสารไม่ควบคุม**  
*J. K. K.*

**Cert. No. : ACL24159**  
**Job No. : VC67AC0071**  
**Pages : 5 of 8**

#### 4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency ( Hz )	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	0.0	-0.1	-0.1	±1.0
125	0.0	0.1	0.0	±1.0
250	0.0	0.0	0.0	±1.0
500	0.0	0.1	0.0	±1.0
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.1	0.0	±1.0
4000	0.0	0.0	0.0	±1.0
8000	0.0	0.1	0.1	+ 1.5, - 2.5
16000	0.0	-1.2	-1.1	+ 2.5, -16.0

#### 5. Frequency and time weightings at 1 kHz

##### 5.1 Frequency weightings at 1 kHz

Frequency Weighting	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	94.0	94.0	0.0	± 0.2
C - weight	94.0	94.0	0.0	± 0.2
Flat	94.0	94.0	0.0	± 0.2

##### 5.2 Time weighting at 1 kHz

Frequency Weighting	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Fast	94.0	94.0	0.0	± 0.1
Slow	94.0	94.0	0.0	± 0.1
Leq	94.0	94.0	0.0	± 0.1

#### 6. Long - term stability

Frequency Weighting	SLM Display at initial ( dB )	SLM Display at final ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	94.0	94.1	0.1	± 0.1

เอกสารไม่ควบคุม

T. Kewin

# SITHIPORN ASSOCIATES CO., LTD.

## CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbunru, Bangplud, Bangkok, 10700 Thailand  
Tel. +66 2433 8331 Email : calibration@sithiporn.com

SITHIPORN  
associates



Cert. No. : ACL24159

Job No. : VC67AC0071

Pages : 6 of 8

### 7. Level linearity on the reference level range

Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
137.0	137.0	0.0	±0.8
136.0	136.0	0.0	±0.8
135.0	135.0	0.0	±0.8
134.0	134.0	0.0	±0.8
133.0	133.0	0.0	±0.8
132.0	132.0	0.0	±0.8
131.0	131.0	0.0	±0.8
129.0	129.0	0.0	±0.8
124.0	124.0	0.0	±0.8
119.0	119.0	0.0	±0.8
114.0	114.0	0.0	±0.8
109.0	109.0	0.0	±0.8
104.0	104.0	0.0	±0.8
99.0	99.0	0.0	±0.8
94.0	94.0	0.0	±0.8
89.0	89.0	0.0	±0.8
84.0	84.0	0.0	±0.8
79.0	79.0	0.0	±0.8
74.0	74.0	0.0	±0.8
69.0	69.0	0.0	±0.8
64.0	64.0	0.0	±0.8
59.0	59.0	0.0	±0.8
54.0	54.0	0.0	±0.8
49.0	49.0	0.0	±0.8
44.0	44.0	0.0	±0.8
39.0	39.0	0.0	±0.8
34.0	34.0	0.0	±0.8
30.0	29.9	-0.1	±0.8
29.0	28.9	-0.1	±0.8
28.0	27.9	-0.1	±0.8
27.0	26.9	-0.1	±0.8
26.0	25.9	-0.1	±0.8
25.0	24.9	-0.1	±0.8

เอกสารไม่ควบคุม  
*F. K. W.*



**Cert. No. : ACL24159**  
**Job No. : VC67AC0071**  
**Pages : 7 of 8**

**8. Level linearity including the level range control**

Range	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Auto	94.0	94.0	0.0	±0.8

**9. Tone burst response**

Time Weighting	Tone burst duration, Tb ( ms )	Cycle	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Fast	0.25	1	108.0	107.9	-0.1	1.0 ; -3.0
	2	8	117.0	117.0	0.0	1.0 ; -1.5
	200	800	134.0	134.1	0.1	±0.5
Slow	2	8	108.0	108.0	0.0	1.0 ; -3.0
	200	800	127.6	127.6	0.0	±0.5
SEL	0.25	1	99.0	98.9	-0.1	1.0 ; -3.0
	2	8	108.0	108.0	0.0	1.0 ; -1.5
	200	800	128.0	128.1	0.1	±0.5

**10. Peak C sound level**

Number of cycle in test signal	Anticipated Value ( dB )	Measured Value, Lcpeak ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Continuous	133.0	133.0	0.0	±2.0
One	136.4	136.4	0.0	±2.0

Number of cycle in test signal	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Continuous	133.0	133.1	0.1	±1.0
Positive half cycle	135.4	135.2	-0.2	±1.0
Negative half cycle	135.4	135.2	-0.2	±1.0

**เอกสารไม่ควบคุม**  
*T. Ketcha*

# SITHIPORN ASSOCIATES CO., LTD. CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand  
Tel. +66 2433 8331 Email : calibration@sithiporn.com

SITHIPORN  
associates



Cert. No. : ACL24159  
Job No. : VC67AC0071  
Pages : 8 of 8

## 11. Overload indication

Measured value ( dB )		Deviated Value ( dB )	Acceptance Limits ( dB )
Positive one-half cycle	Negative one-half cycle		
89.5	89.6	0.1	±1.5

## 12. High level stability

Frequency Weighting	SLM Display at initial ( dB )	SLM Display at final ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	137.0	136.9	0.1	±0.1

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor  $k = 2$   
or any value following calculation, providing a level of confidence of approximately 95 %

————— **End of Calibration Certificate** —————

เอกสารไม่ควบคุม  
*T. Ketcha*

Cert. No. : ACL24054

Pages : 1 of 8

## Calibration Certificate

**Equipment :** SOUND LEVEL METER  
**Manufacturer :** RION  
**Model :** NL-42 / Microphone UC-52 / Preamplifier NH-24  
**Serial No.:** 00409109 / 189688 / 90554  
**ID No.:** UAE.EFM.013/2564

**Condition As Found :** GOOD

**Customer :** UNITED ANALYST AND ENGINEERING CONSULTANT (UAE)  
81 SOI UDOMSUK 41, SUKHUMVIT ROAD,  
BANGCHAK SUB-DISTRICT,  
PHRAKHANONG DISTRICT, BANGKOK 10260  
THAILAND.

**Location :** -

**Ambient Temperature :** ( 23.0  $\pm$  3 ) °C  
**Pressure :** ( 101.3  $\pm$  3 ) kPa  
**Relative Humidity :** ( 50.0  $\pm$  20 ) %

**Received Date :** 21 DECEMBER 2023  
**Calibration Date :** 18-19 JANUARY 2024  
**Date of Issue :** 22 JANUARY 2024

**Calibrated by :**

Nathakorn Pisutpaisan

**Approved by :**

  
( Thanakul Petchurai )

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

เอกสารไม่ควบคุม

# SITHIPORN ASSOCIATES CO., LTD. CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand  
Tel. +66 2433 8331 Email : calibration@sithiporn.com

SITHIPORN  
associates



Cert. No. : ACL24054  
Job No. : VC67AC0034  
Pages : 2 of 8

Calibration Procedure : CP-AC-01

## Calibration Method :

This equipment was calibrated by follow on IEC-61672-3 (2013) Standard for sound level meter (SLM).

The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.

For tests results of each items were made by observation of each Instruments display and also with SLM's display.

## Condition of this result of calibration :

### 1. Reference Standard Instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
Waveform Generator	33210A	MY48017076	EF-0009-23	07-FEB-24
Waveform Generator	33511B	MY52302742	EF-0010-23	07-FEB-24
Digital Multimeter	33461A	MY53220104	EEL.BP 30/0266	13-FEB-24
Digital Multimeter	33461A	MY53220076	EEL.BP 29/0266	13-FEB-24
Digital Multimeter	34461A	MY60024273	EEL.BP 31/0266	14-FEB-24
Programmable Attenuator	MAT-1070	62100114	EF-0011-23	08-FEB-24
Condenser Microphone	4180	2977900	AA-1001-23	14-FEB-24
Measuring Amplifier	NA-42KAI	34560495	AA-3002-23	14-FEB-24

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is traceable to the international system of unit maintained at :

3.1 National Institute of Metrology (Thailand).

3.2 Thailand Institute of Scientific and Technological Research (TISTR).

เอกสารไม่ควบคุม

*[Signature]*



# SITHIPORN ASSOCIATES CO., LTD. CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand  
Tel. +66 2433 8331 Email : calibration@sithiporn.com

SITHIPORN  
associates



Cert. No. : ACL24054

Job No. : VC67AC0034

Pages : 3 of 8

## Summary of Measurement Result :

Parameter	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	0.2	N/A
2. Self-generated noise	0.2	N/A
3. Acoustical signal tests of frequency weightings		
125 Hz	0.3	0.6
1000 Hz	0.3	0.6
8000 Hz	0.3	0.7
4. Electrical signal tests of frequency weightings		
For 10 Hz to 4 kHz	0.3	0.6
For > 4 kHz to 10 kHz	0.3	0.7
For > 10 kHz to 20 kHz	-	1.0
5. Frequency and time weightings at 1 kHz	0.2	0.2
6. Long - term stability	0.1	0.1
7. Level linearity on the reference level range	0.2	0.3
8. Level linearity including the level range control	0.2	0.3
9. Tone burst response	0.2	0.3
10. Peak C sound level	0.2	0.35
11. Overload indication	0.2	0.25
12. High level stability	0.1	0.1

เอกสารไม่ควบคุม  
T. Kewin

# SITHIPORN ASSOCIATES CO., LTD.

## CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand  
Tel. +66 2433 8331 Email : calibration@sithiporn.com

SITHIPORN  
associates



Cert. No. : ACL24054

Job No. : VC67AC0034

Pages : 4 of 8

### Result of calibration :

#### 1. Absolute sensitivity

Reference Acoustic Signal ( dB )	Measured Value ( dB )	Deviation ( dB )	Acceptance Limit ( dB )
93.9 (93.98)	93.9	0.0	±0.3

#### 2. Self-generated noise

##### 2.1 Normal test

Measured Value ( dB )
15.7

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Measured value ( dB )
A - weight	12.0
C - weight	18.2
Flat	24.0

#### 3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency ( Hz )	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
125	0.0	0.0	0.0	± 1.5
1000	0.0	0.0	0.0	± 1.0
8000	2.5	2.6	2.6	±5.0

เอกสารไม่ควบคุม  
T. Kewin

**Cert. No. : ACL24054**  
**Job No. : VC67AC0034**  
**Pages : 5 of 8**

#### 4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency ( Hz )	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	0.0	0.0	0.0	±2.0
125	0.0	0.0	0.0	±1.5
250	0.0	0.0	0.0	±1.5
500	0.0	0.0	0.0	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.1	0.0	±2.0
4000	0.0	0.0	0.0	±3.0
8000	0.0	0.1	0.1	±5.0

#### 5. Frequency and time weightings at 1 kHz

##### 5.1 Frequency weightings at 1 kHz

Frequency Weighting	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	94.0	94.0	0.0	± 0.2
C - weight	94.0	94.0	0.0	± 0.2
Flat	94.0	94.0	0.0	± 0.2

##### 5.2 Time weighting at 1 kHz

Frequency Weighting	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Fast	94.0	94.0	0.0	± 0.1
Slow	94.0	94.0	0.0	± 0.1
Leq	94.0	94.0	0.0	± 0.1

#### 6. Long - term stability

Frequency Weighting	SLM Display at initial ( dB )	SLM Display at final ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	94.0	94.0	0.0	± 0.3

**เอกสารไม่ควบคุม**  
*T. Kewin.*

# SITHIPORN ASSOCIATES CO., LTD. CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand  
Tel. +66 2433 8331 Email : calibration@sithiporn.com

SITHIPORN  
associates



Cert. No. : ACL24054

Job No. : VC67AC0034

Pages : 6 of 8

## 7. Level linearity on the reference level range

Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
137.0	137.0	0.0	$\pm 1.1$
136.0	136.0	0.0	$\pm 1.1$
135.0	135.0	0.0	$\pm 1.1$
134.0	134.0	0.0	$\pm 1.1$
133.0	133.0	0.0	$\pm 1.1$
132.0	132.0	0.0	$\pm 1.1$
131.0	131.0	0.0	$\pm 1.1$
129.0	129.0	0.0	$\pm 1.1$
124.0	124.0	0.0	$\pm 1.1$
119.0	119.0	0.0	$\pm 1.1$
114.0	114.0	0.0	$\pm 1.1$
109.0	109.0	0.0	$\pm 1.1$
104.0	104.0	0.0	$\pm 1.1$
99.0	99.0	0.0	$\pm 1.1$
94.0	94.0	0.0	$\pm 1.1$
89.0	89.0	0.0	$\pm 1.1$
84.0	84.0	0.0	$\pm 1.1$
79.0	79.0	0.0	$\pm 1.1$
74.0	74.0	0.0	$\pm 1.1$
69.0	69.0	0.0	$\pm 1.1$
64.0	64.0	0.0	$\pm 1.1$
59.0	59.0	0.0	$\pm 1.1$
54.0	54.0	0.0	$\pm 1.1$
49.0	49.0	0.0	$\pm 1.1$
44.0	44.0	0.0	$\pm 1.1$
39.0	38.9	-0.1	$\pm 1.1$
34.0	34.0	0.0	$\pm 1.1$
30.0	29.9	-0.1	$\pm 1.1$
29.0	28.9	-0.1	$\pm 1.1$
28.0	27.9	-0.1	$\pm 1.1$
27.0	26.9	-0.1	$\pm 1.1$
26.0	25.9	-0.1	$\pm 1.1$
25.0	24.9	-0.1	$\pm 1.1$

เอกสารไม่ควบคุม  
7. Kel...



# SITHIPORN ASSOCIATES CO., LTD. CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand  
Tel. +66 2433 8331 Email : calibration@sithiporn.com

SITHIPORN  
associates



Cert. No. : ACL24054  
Job No. : VC67AC0034  
Pages : 7 of 8

## 8. Level linearity including the level range control

Range	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Auto	94.0	94.0	0.0	±1.1

## 9. Tone burst response

Time Weighting	Tone burst duration, Tb ( ms )	Cycle	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.1	0.1	±1.0
Slow	2	8	108.0	108.0	0.0	1.5 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
SEL	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.1	0.1	±1.0

## 10. Peak C sound level

Number of cycle in test signal	Anticipated Value ( dB )	Measured Value, Lcpeak ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Continuous	133.0	133.0	0.0	±3.0
One	136.4	135.6	-0.8	±3.0

Number of cycle in test signal	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Continuous	133.0	133.0	0.0	±2.0
Positive half cycle	135.4	135.2	-0.2	±2.0
Negative half cycle	135.4	135.2	-0.2	±2.0

เอกสารไม่ควบคุม  
T. Kelwan

# SITHIPORN ASSOCIATES CO., LTD.

## CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand  
Tel. +66 2433 8331 Email : calibration@sithiporn.com

SITHIPORN  
associates



Cert. No. : ACL24054  
Job No. : VC67AC0034  
Pages : 8 of 8

### 11. Overload indication

Measured value ( dB )		Deviated Value ( dB )	Acceptance Limits ( dB )
Positive one-half cycle	Negative one-half cycle		
89.5	89.7	0.2	±1.5

### 12. High level stability

Frequency Weighting	SLM Display at initial ( dB )	SLM Display at final ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor  $k = 2$   
or any value following calculation, providing a level of confidence of approximately 95 %

————— End of Calibration Certificate —————

เอกสารไม่ควบคุม  
7. Ketch

Cert. No. : ACL24157

Pages : 1 of 8

## Calibration Certificate

**Equipment :** SOUND LEVEL METER  
**Manufacturer :** RION  
**Model :** NL-42 / Microphone UC-52 / Preamplifier NH-24  
**Serial No.:** 01010778 / 194533 / 14656  
**ID No.:** UAE.EFM.081/2565

**Condition As Found :** GOOD

**Customer :** UNITED ANALYST AND ENGINEERING CONSULTANT (UAE)  
81 SOI UDOMSUK 41, SUKHUMVIT ROAD,  
BANGCHAK SUB-DISTRICT,  
PHRAKHANONG DISTRICT, BANGKOK 10260  
THAILAND.

**Location :** -

**Ambient Temperature :** ( 23.0  $\pm$  3 ) °C  
**Pressure :** ( 101.3  $\pm$  3 ) kPa  
**Relative Humidity :** ( 50.0  $\pm$  20 ) %

**Received Date :** 10 MAY 2024  
**Calibration Date :** 30 - 31 MAY 2024  
**Date of Issue :** 04 JUNE 2024

**Calibrated by :** Nathakorn Pisutpaisan

**Approved by :**

  
( Thanakul Petchurai )

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

เอกสารไม่ควบคุม

# SITHIPORN ASSOCIATES CO., LTD. CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand  
Tel. +66 2433 8331 Email : calibration@sithiporn.com



Cert. No. : ACL24157  
Job No. : VC67AC0071  
Pages : 2 of 8

Calibration Procedure : CP-AC-01

## Calibration Method :

This equipment was calibrated by follow on IEC-61672-3 (2013) Standard for sound level meter (SLM).

The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.

For tests results of each items were made by observation of each Instruments display and also with SLM's display.

## Condition of this result of calibration :

### 1. Reference Standard Instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
Waveform Generator	33210A	MY48017076	EF-0009-24	05-FEB-25
Waveform Generator	33511B	MY52302742	EF-0007-24	05-FEB-25
Digital Multimeter	33461A	MY53220104	EEL.BP 21/0267	13-FEB-25
Digital Multimeter	33461A	MY53220076	EEL.BP 20/0267	15-FEB-25
Digital Multimeter	34461A	MY60024273	EEL.BP 22/0267	15-FEB-25
Programmable Attenuator	MAT-1070	62100114	EF-0008-24	05-FEB-25
Condenser Microphone	4180	2977900	AA-1001-24	12-FEB-25
Measuring Amplifier	NA-42KAI	34560495	AA-3001-24	05-FEB-25

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is traceable to the international system of unit maintained at :

3.1 National Institute of Metrology (Thailand).

3.2 Thailand Institute of Scientific and Technological Research (TISTR).

เอกสารไม่ควบคุม  
7. Rekh-



# SITHIPORN ASSOCIATES CO., LTD. CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand  
Tel. +66 2433 8331 Email : calibration@sithiporn.com

SITHIPORN  
associates



Cert. No. : ACL24157  
Job No. : VC67AC0071  
Pages : 3 of 8

## Summary of Measurement Result :

Parameter	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	0.2	N/A
2. Self-generated noise	0.2	N/A
3. Acoustical signal tests of frequency weightings		
125 Hz	0.3	0.6
1000 Hz	0.3	0.6
8000 Hz	0.3	0.7
4. Electrical signal tests of frequency weightings		
For 10 Hz to 4 kHz	0.3	0.6
For > 4 kHz to 10 kHz	0.3	0.7
For > 10 kHz to 20 kHz	-	1.0
5. Frequency and time weightings at 1 kHz	0.2	0.2
6. Long - term stability	0.1	0.1
7. Level linearity on the reference level range	0.2	0.3
8. Level linearity including the level range control	0.2	0.3
9. Tone burst response	0.2	0.3
10. Peak C sound level	0.2	0.35
11. Overload indication	0.2	0.25
12. High level stability	0.1	0.1

เอกสารไม่ควบคุม  
*G. K. K.*

**Cert. No. : ACL24157**

**Job No. : VC67AC0071**

**Pages : 4 of 8**

**Result of calibration :**

**1. Absolute sensitivity**

Reference Acoustic Signal ( dB )	Measured Value ( dB )	Deviation ( dB )	Acceptance Limit ( dB )
93.9 (93.94)	93.9	0.0	±0.3

**2. Self-generated noise**

**2.1 Normal test**

Measured Value ( dB )
14.7

**2.2 The microphone of the sound level meter was replaced by electrical signal input device.**

Frequency Weighting	Measured value ( dB )
A - weight	11.2
C - weight	17.5
Flat	23.1

**3. Acoustical signal tests of frequency weightings**

Meter free-field acoustic response at a level of 84 dB

Frequency ( Hz )	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
125	0.1	0.1	0.1	± 1.5
1000	0.0	0.0	0.0	± 1.0
8000	0.5	0.6	0.6	±5.0

**Cert. No. : ACL24157**  
**Job No. : VC67AC0071**  
**Pages : 5 of 8**

#### 4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency ( Hz )	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	-0.1	0.0	-0.1	±2.0
125	0.0	0.1	0.0	±1.5
250	0.0	0.0	0.0	±1.5
500	0.0	0.1	0.0	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.1	0.1	±2.0
4000	0.0	0.1	0.0	±3.0
8000	0.1	0.1	0.1	±5.0

#### 5. Frequency and time weightings at 1 kHz

##### 5.1 Frequency weightings at 1 kHz

Frequency Weighting	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	94.0	94.0	0.0	± 0.2
C - weight	94.0	94.0	0.0	± 0.2
Flat	94.0	94.0	0.0	± 0.2

##### 5.2 Time weighting at 1 kHz

Frequency Weighting	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Fast	94.0	94.0	0.0	± 0.1
Slow	94.0	94.0	0.0	± 0.1
Leq	94.0	94.0	0.0	± 0.1

#### 6. Long - term stability

Frequency Weighting	SLM Display at initial ( dB )	SLM Display at final ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	94.0	94.1	0.1	

เอกสารไม่ควบคุม

T. Kehn

# SITHIPORN ASSOCIATES CO., LTD. CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand  
Tel. +66 2433 8331 Email : calibration@sithiporn.com

SITHIPORN  
associates



Cert. No. : ACL24157

Job No. : VC67AC0071

Pages : 6 of 8

## 7. Level linearity on the reference level range

Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
137.0	137.0	0.0	$\pm 1.1$
136.0	136.0	0.0	$\pm 1.1$
135.0	135.1	0.1	$\pm 1.1$
134.0	134.1	0.1	$\pm 1.1$
133.0	133.0	0.0	$\pm 1.1$
132.0	132.0	0.0	$\pm 1.1$
131.0	131.0	0.0	$\pm 1.1$
129.0	129.0	0.0	$\pm 1.1$
124.0	124.0	0.0	$\pm 1.1$
119.0	119.1	0.1	$\pm 1.1$
114.0	114.0	0.0	$\pm 1.1$
109.0	109.0	0.0	$\pm 1.1$
104.0	104.1	0.1	$\pm 1.1$
99.0	99.0	0.0	$\pm 1.1$
94.0	94.0	0.0	$\pm 1.1$
89.0	89.0	0.0	$\pm 1.1$
84.0	84.0	0.0	$\pm 1.1$
79.0	79.0	0.0	$\pm 1.1$
74.0	74.0	0.0	$\pm 1.1$
69.0	69.0	0.0	$\pm 1.1$
64.0	64.0	0.0	$\pm 1.1$
59.0	59.0	0.0	$\pm 1.1$
54.0	54.0	0.0	$\pm 1.1$
49.0	49.0	0.0	$\pm 1.1$
44.0	44.0	0.0	$\pm 1.1$
39.0	39.0	0.0	$\pm 1.1$
34.0	34.0	0.0	$\pm 1.1$
30.0	30.0	0.0	$\pm 1.1$
29.0	29.1	0.1	$\pm 1.1$
28.0	28.1	0.1	$\pm 1.1$
27.0	27.2	0.2	$\pm 1.1$
26.0	26.3	0.3	$\pm 1.1$
25.0	25.4	0.4	$\pm 1.1$

เอกสารไม่ควบคุม  
F. Ketchu



# SITHIPORN ASSOCIATES CO., LTD. CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand  
Tel. +66 2433 8331 Email : calibration@sithiphorn.com

SITHIPORN  
associates



Cert. No. : ACL24157  
Job No. : VC67AC0071  
Pages : 7 of 8

## 8. Level linearity including the level range control

Range	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Auto	94.0	94.0	0.0	±1.1

## 9. Tone burst response

Time Weighting	Tone burst duration, Tb ( ms )	Cycle	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	116.9	-0.1	1.0 ; -2.5
	200	800	134.0	134.0	0.0	±1.0
Slow	2	8	108.0	107.9	-0.1	1.5 ; -5.0
	200	800	127.6	127.5	-0.1	±1.0
SEL	0.25	1	99.0	98.8	-0.2	1.5 ; -5.0
	2	8	108.0	107.9	-0.1	1.0 ; -2.5
	200	800	128.0	128.0	0.0	±1.0

## 10. Peak C sound level

Number of cycle in test signal	Anticipated Value ( dB )	Measured Value, Lcpeak ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Continuous	133.0	133.0	0.0	±3.0
One	136.4	135.6	-0.8	±3.0

Number of cycle in test signal	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Continuous	133.0	132.9	-0.1	±2.0
Positive half cycle	135.4	135.1	-0.3	±2.0
Negative half cycle	135.4	135.1	-0.3	±2.0

เอกสารไม่ควบคุม  
T. Ketkarn

# SITHIPORN ASSOCIATES CO., LTD. CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand  
Tel. +66 2433 8331 Email : calibration@sithiporn.com

SITHIPORN  
associates



Cert. No. : ACL24157  
Job No. : VC67AC0071  
Pages : 8 of 8

## 11. Overload indication

Measured value ( dB )		Deviated Value ( dB )	Acceptance Limits ( dB )
Positive one-half cycle	Negative one-half cycle		
89.5	89.6	0.1	±1.5

## 12. High level stability

Frequency Weighting	SLM Display at initial ( dB )	SLM Display at final ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor  $k = 2$   
or any value following calculation, providing a level of confidence of approximately 95 %

————— End of Calibration Certificate —————

เอกสารไม่ควบคุม  
*T. Ketchu*

Cert. No. : ACL24065

Pages : 1 of 8

## Calibration Certificate

**Equipment :** SOUND LEVEL METER  
**Manufacturer :** RION  
**Model :** NL-62 / Microphone UC-59L / Preamplifier NH-26  
**Serial No.:** 00881367 / 01639 / 01457  
**ID No.:** UAE.EFM.027/2564

**Condition As Found :** GOOD

**Customer :** UNITED ANALYST AND ENGINEERING CONSULTANT (UAE)  
81 SOI UDOMSUK 41, SUKHUMVIT ROAD,  
BANGCHAK SUB-DISTRICT,  
PHRAKHANONG DISTRICT, BANGKOK 10260  
THAILAND.

**Location :** -

**Ambient Temperature :** ( 23.0  $\pm$  3 ) °C  
**Pressure :** ( 101.3  $\pm$  3 ) kPa  
**Relative Humidity :** ( 50.0  $\pm$  20 ) %

**Received Date :** 21 DECEMBER 2023  
**Calibration Date :** 18-19 JANUARY 2024  
**Date of Issue :** 22 JANUARY 2024

**Calibrated by :**

Nathakorn Pisutpaisan

**Approved by :**

*T. Petchurai*  
( Thanakul Petchurai )

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

เอกสารควบคุม

# SITHIPORN ASSOCIATES CO., LTD.

## CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand  
Tel. +66 2433 8331 Email : calibration@sithiporn.com

SITHIPORN  
associates



Cert. No. : ACL24065

Job No. : VC67AC0034

Pages : 2 of 8

Calibration Procedure : CP-AC-01

### Calibration Method :

This equipment was calibrated by follow on IEC-61672-3 (2013) Standard for sound level meter (SLM).

The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.

For tests results of each items were made by observation of each Instruments display and also with SLM's display.

### Condition of this result of calibration :

#### 1. Reference Standard Instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
Waveform Generator	33210A	MY48017076	EF-0009-23	07-FEB-24
Waveform Generator	33511B	MY52302742	EF-0010-23	07-FEB-24
Digital Multimeter	33461A	MY53220104	EEL.BP 30/0266	13-FEB-24
Digital Multimeter	33461A	MY53220076	EEL.BP 29/0266	13-FEB-24
Digital Multimeter	34461A	MY60024273	EEL.BP 31/0266	14-FEB-24
Programmable Attenuator	MAT-1070	62100114	EF-0011-23	08-FEB-24
Condenser Microphone	4180	2977900	AA-1001-23	14-FEB-24
Measuring Amplifier	NA-42KAI	34560495	AA-3002-23	14-FEB-24

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is traceable to the international system of unit maintained at :

3.1 National Institute of Metrology (Thailand).

3.2 Thailand Institute of Scientific and Technological Research (TISTR).

เอกสารควบคุม



# SITHIPORN ASSOCIATES CO., LTD.

## CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand  
Tel. +66 2433 8331 Email : calibration@sithiporn.com

SITHIPORN  
associates



Cert. No. : ACL24065  
Job No. : VC67AC0034  
Pages : 3 of 8

### Summary of Measurement Result :

Parameter	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	0.2	N/A
2. Self-generated noise	0.3	N/A
3. Acoustical signal tests of frequency weightings		
125 Hz	0.3	0.6
1000 Hz	0.3	0.6
8000 Hz	0.3	0.7
4. Electrical signal tests of frequency weightings		
For 10 Hz to 4 kHz	0.3	0.6
For > 4 kHz to 10 kHz	0.3	0.7
For > 10 kHz to 20 kHz	0.3	1.0
5. Frequency and time weightings at 1 kHz	0.2	0.2
6. Long - term stability	0.1	0.1
7. Level linearity on the reference level range	0.2	0.3
8. Level linearity including the level range control	0.2	0.3
9. Tone burst response	0.2	0.3
10. Peak C sound level	0.2	0.35
11. Overload indication	0.2	0.25
12. High level stability	0.1	0.1

เอกสารควบคุม

# SITHIPORN ASSOCIATES CO., LTD.

## CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand  
Tel. +66 2433 8331 Email : calibration@sithiporn.com

SITHIPORN  
associates



Cert. No. : ACL24065

Job No. : VC67AC0034

Pages : 4 of 8

### Result of calibration :

#### 1. Absolute sensitivity

Reference Acoustic Signal ( dB )	Measured Value ( dB )	Deviation ( dB )	Acceptance Limit ( dB )
93.9 (93.98)	94.0	0.0	±0.3

#### 2. Self-generated noise

##### 2.1 Normal test

Measured Value ( dB )
19.0

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Measured value ( dB )
A - weight	13.0
C - weight	18.0
Flat	25.3

#### 3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency ( Hz )	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
125	0.0	0.1	0.1	± 1.0
1000	0.1	0.1	0.1	± 0.7
8000	1.2	1.3	1.3	+ 1.5, - 2.5

เอกสารควบคุม

Cert. No. : ACL24065  
 Job No. : VC67AC0034  
 Pages : 5 of 8

#### 4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency ( Hz )	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	0.0	-0.1	-0.1	±1.0
125	0.0	0.0	0.0	±1.0
250	0.0	0.0	0.0	±1.0
500	0.0	0.0	0.0	±1.0
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.0	0.0	±1.0
4000	0.0	0.0	0.0	±1.0
8000	0.0	0.0	0.0	+ 1.5, - 2.5
16000	0.0	-1.2	-1.2	+ 2.5, -16.0

#### 5. Frequency and time weightings at 1 kHz

##### 5.1 Frequency weightings at 1 kHz

Frequency Weighting	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	94.0	94.0	0.0	± 0.2
C - weight	94.0	94.0	0.0	± 0.2
Flat	94.0	94.0	0.0	± 0.2

##### 5.2 Time weighting at 1 kHz

Frequency Weighting	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Fast	94.0	94.0	0.0	± 0.1
Slow	94.0	94.0	0.0	± 0.1
Leq	94.0	94.0	0.0	± 0.1

#### 6. Long - term stability

Frequency Weighting	SLM Display at initial ( dB )	SLM Display at final ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	94.0	94.0	0.0	± 0.1

# SITHIPORN ASSOCIATES CO., LTD.

## CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand  
Tel. +66 2433 8331 Email : calibration@sithiporn.com

SITHIPORN  
associates



Cert. No. : ACL24065

Job No. : VC67AC0034

Pages : 6 of 8

### 7. Level linearity on the reference level range

Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
137.0	137.1	0.1	±0.8
136.0	136.1	0.1	±0.8
135.0	135.1	0.1	±0.8
134.0	134.1	0.1	±0.8
133.0	133.1	0.1	±0.8
132.0	132.1	0.1	±0.8
131.0	131.0	0.0	±0.8
129.0	129.1	0.1	±0.8
124.0	124.0	0.0	±0.8
119.0	119.1	0.1	±0.8
114.0	114.1	0.1	±0.8
109.0	109.1	0.1	±0.8
104.0	104.1	0.1	±0.8
99.0	99.1	0.1	±0.8
94.0	94.0	0.0	±0.8
89.0	89.0	0.0	±0.8
84.0	84.0	0.0	±0.8
79.0	79.0	0.0	±0.8
74.0	74.0	0.0	±0.8
69.0	69.0	0.0	±0.8
64.0	64.0	0.0	±0.8
59.0	59.0	0.0	±0.8
54.0	54.0	0.0	±0.8
49.0	49.0	0.0	±0.8
44.0	44.0	0.0	±0.8
39.0	39.0	0.0	±0.8
34.0	34.0	0.0	±0.8
30.0	29.9	-0.1	±0.8
29.0	28.9	-0.1	±0.8
28.0	28.0	0.0	±0.8
27.0	26.9	-0.1	±0.8
26.0	25.9	-0.1	±0.8
25.0	24.9	-0.1	±0.8

เอกสารควบคุม



# SITHIPORN ASSOCIATES CO., LTD.

## CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbunru, Bangplud, Bangkok, 10700 Thailand  
Tel. +66 2433 8331 Email : calibration@sithiporn.com

SITHIPORN  
associates



Cert. No. : ACL24065  
Job No. : VC67AC0034  
Pages : 7 of 8

### 8. Level linearity including the level range control

Range	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Auto	94.0	94.0	0.0	±0.8

### 9. Tone burst response

Time Weighting	Tone burst duration, Tb ( ms )	Cycle	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Fast	0.25	1	108.0	107.9	-0.1	1.0 ; -3.0
	2	8	117.0	117.0	0.0	1.0 ; -1.5
	200	800	134.0	134.0	0.0	±0.5
Slow	2	8	108.0	108.0	0.0	1.0 ; -3.0
	200	800	127.6	127.6	0.0	±0.5
SEL	0.25	1	99.0	98.9	-0.1	1.0 ; -3.0
	2	8	108.0	108.0	0.0	1.0 ; -1.5
	200	800	128.0	128.0	0.0	±0.5

### 10. Peak C sound level

Number of cycle in test signal	Anticipated Value ( dB )	Measured Value, Lcpeak ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Continuous	133.0	133.0	0.0	±2.0
One	136.4	135.3	-1.1	±2.0

Number of cycle in test signal	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Continuous	133.0	133.0	0.0	±1.0
Positive half cycle	135.4	135.1	-0.3	±1.0
Negative half cycle	135.4	135.1	-0.3	±1.0

เอกสารควบคุม

# SITHIPORN ASSOCIATES CO., LTD. CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbunru, Bangplud, Bangkok, 10700 Thailand  
Tel. +66 2433 8331 Email : calibration@sithiporn.com

SITHIPORN  
associates



Cert. No. : ACL24065  
Job No. : VC67AC0034  
Pages : 8 of 8

## 11. Overload indication

Measured value ( dB )		Deviated Value ( dB )	Acceptance Limits ( dB )
Positive one-half cycle	Negative one-half cycle		
89.4	89.5	0.1	±1.5

## 12. High level stability

Frequency Weighting	SLM Display at initial ( dB )	SLM Display at final ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	137.0	137.0	0.0	±0.1

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor  $k = 2$   
or any value following calculation, providing a level of confidence of approximately 95 %

————— End of Calibration Certificate —————

เอกสารควบคุม

Cert. No. : ACL24100

Pages : 1 of 8

## Calibration Certificate

**Equipment :** SOUND LEVEL METER  
**Manufacturer :** RION  
**Model :** NL-42 / Microphone UC-52 / Preamplifier NH-24  
**Serial No.:** 00558212 / 157973 / 48067  
**ID No.:** UAE.EFM.044/2558

**Condition As Found :** GOOD

**Customer :** UNITED ANALYST AND ENGINEERING CONSULTANT (UAE)  
81 SOI UDOMSUK 41, SUKHUMVIT ROAD,  
BANGCHAK SUB-DISTRICT,  
PHRAKHANONG DISTRICT, BANGKOK 10260  
THAILAND.

**Location :** -  
**Ambient Temperature :** ( 23.0  $\pm$  3 ) °C  
**Pressure :** ( 101.3  $\pm$  3 ) kPa  
**Relative Humidity :** ( 50.0  $\pm$  20 ) %

**Received Date :** 18 JANUARY 2024  
**Calibration Date :** 29-30 JANUARY 2024  
**Date of Issue :** 02 FEBRUARY 2024

**Calibrated by :** Nathakorn Pisutpaisan

**Approved by :**

  
( Thanakul Petchurai )

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

เอกสารไม่ควบคุม

# SITHIPORN ASSOCIATES CO., LTD.

## CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand  
Tel. +66 2433 8331 Email : calibration@sithiporn.com



Cert. No. : ACL24100  
Job No. : VC67AC0057  
Pages : 2 of 8

Calibration Procedure : CP-AC-01

### Calibration Method :

This equipment was calibrated by follow on IEC-61672-3 (2013) Standard for sound level meter (SLM).

The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.

For tests results of each items were made by observation of each Instruments display and also with SLM's display.

### Condition of this result of calibration :

#### 1. Reference Standard Instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
Waveform Generator	33210A	MY48017076	EF-0009-23	07-FEB-24
Waveform Generator	33511B	MY52302742	EF-0010-23	07-FEB-24
Digital Multimeter	33461A	MY53220104	EEL.BP 30/0266	13-FEB-24
Digital Multimeter	33461A	MY53220076	EEL.BP 29/0266	13-FEB-24
Digital Multimeter	34461A	MY60024273	EEL.BP 31/0266	14-FEB-24
Programmable Attenuator	MAT-1070	62100114	EF-0011-23	08-FEB-24
Condenser Microphone	4180	2977900	AA-1001-23	14-FEB-24
Measuring Amplifier	NA-42KAI	34560495	AA-3002-23	14-FEB-24

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is traceable to the international system of unit maintained at :

3.1 National Institute of Metrology (Thailand).

3.2 Thailand Institute of Scientific and Technological Research (TISTR).

เอกสารไม่ควบคุม  
Y. Ketcha



# SITHIPORN ASSOCIATES CO., LTD.

## CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand  
Tel. +66 2433 8331 Email : calibration@sithiporn.com

SITHIPORN  
associates



Cert. No. : ACL24100  
Job No. : VC67AC0057  
Pages : 3 of 8

### Summary of Measurement Result :

Parameter	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	0.2	N/A
2. Self-generated noise	0.2	N/A
3. Acoustical signal tests of frequency weightings		
125 Hz	0.3	0.6
1000 Hz	0.3	0.6
8000 Hz	0.3	0.7
4. Electrical signal tests of frequency weightings		
For 10 Hz to 4 kHz	0.3	0.6
For > 4 kHz to 10 kHz	0.3	0.7
For > 10 kHz to 20 kHz	-	1.0
5. Frequency and time weightings at 1 kHz	0.2	0.2
6. Long - term stability	0.1	0.1
7. Level linearity on the reference level range	0.2	0.3
8. Level linearity including the level range control	0.2	0.3
9. Tone burst response	0.2	0.3
10. Peak C sound level	0.2	0.35
11. Overload indication	0.2	0.25
12. High level stability	0.1	0.1

เอกสารไม่ควบคุม  
*F. Kehn*

# SITHIPORN ASSOCIATES CO., LTD.

## CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand  
Tel. +66 2433 8331 Email : calibration@sithiporn.com

SITHIPORN  
associates



Cert. No. : ACL24100

Job No. : VC67AC0057

Pages : 4 of 8

### Result of calibration :

#### 1. Absolute sensitivity

Reference Acoustic Signal ( dB )	Measured Value ( dB )	Deviation ( dB )	Acceptance Limit ( dB )
93.9 (93.98)	93.9	0.0	±0.3

#### 2. Self-generated noise

##### 2.1 Normal test

Measured Value ( dB )
16.7

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Measured value ( dB )
A - weight	13.4
C - weight	19.3
Flat	25.0

#### 3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency ( Hz )	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
125	0.2	0.2	0.2	± 1.5
1000	0.0	0.0	0.0	± 1.0
8000	1.0	1.1	1.1	±5.0

เอกสารไม่ควบคุม  
F. Kelen

Cert. No. : ACL24100  
 Job No. : VC67AC0057  
 Pages : 5 of 8

#### 4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency ( Hz )	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	0.0	0.0	0.0	±2.0
125	0.0	0.1	0.0	±1.5
250	0.0	0.0	0.0	±1.5
500	0.0	0.1	0.0	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.1	0.0	±2.0
4000	0.0	0.0	0.0	±3.0
8000	0.0	0.1	0.1	±5.0

#### 5. Frequency and time weightings at 1 kHz

##### 5.1 Frequency weightings at 1 kHz

Frequency Weighting	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	94.0	94.0	0.0	± 0.2
C - weight	94.0	94.0	0.0	± 0.2
Flat	94.0	94.0	0.0	± 0.2

##### 5.2 Time weighting at 1 kHz

Frequency Weighting	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Fast	94.0	94.0	0.0	± 0.1
Slow	94.0	94.0	0.0	± 0.1
Leq	94.0	94.0	0.0	± 0.1

#### 6. Long - term stability

Frequency Weighting	SLM Display at initial ( dB )	SLM Display at final ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	94.0	94.0	0.0	± 0.3

เอกสารไม่ควบคุม

7. Relu...

# SITHIPORN ASSOCIATES CO., LTD.

## CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand  
Tel. +66 2433 8331 Email : calibration@sithiporn.com

SITHIPORN  
associates



Cert. No. : ACL24100

Job No. : VC67AC0057

Pages : 6 of 8

### 7. Level linearity on the reference level range

Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
137.0	137.0	0.0	± 1.1
136.0	136.0	0.0	± 1.1
135.0	135.0	0.0	± 1.1
134.0	134.0	0.0	± 1.1
133.0	133.0	0.0	± 1.1
132.0	132.0	0.0	± 1.1
131.0	131.0	0.0	± 1.1
129.0	129.0	0.0	± 1.1
124.0	124.0	0.0	± 1.1
119.0	119.0	0.0	± 1.1
114.0	114.0	0.0	± 1.1
109.0	109.0	0.0	± 1.1
104.0	104.0	0.0	± 1.1
99.0	99.0	0.0	± 1.1
94.0	94.0	0.0	± 1.1
89.0	89.0	0.0	± 1.1
84.0	84.0	0.0	± 1.1
79.0	79.0	0.0	± 1.1
74.0	74.0	0.0	± 1.1
69.0	69.0	0.0	± 1.1
64.0	64.0	0.0	± 1.1
59.0	59.0	0.0	± 1.1
54.0	54.0	0.0	± 1.1
49.0	49.0	0.0	± 1.1
44.0	44.0	0.0	± 1.1
39.0	39.0	0.0	± 1.1
34.0	34.0	0.0	± 1.1
30.0	30.1	0.1	± 1.1
29.0	29.1	0.1	± 1.1
28.0	28.2	0.2	± 1.1
27.0	27.2	0.2	± 1.1
26.0	26.3	0.3	± 1.1
25.0	25.3	0.3	± 1.1

เอกสารไม่ควบคุม  
*[Signature]*



# SITHIPORN ASSOCIATES CO., LTD.

## CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand  
Tel. +66 2433 8331 Email : calibration@sithiporn.com

SITHIPORN  
associates



Cert. No. : ACL24100  
Job No. : VC67AC0057  
Pages : 7 of 8

### 8. Level linearity including the level range control

Range	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Auto	94.0	94.0	0.0	±1.1

### 9. Tone burst response

Time Weighting	Tone burst duration, Tb ( ms )	Cycle	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.1	0.1	±1.0
Slow	2	8	108.0	108.0	0.0	1.5 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
SEL	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.1	0.1	±1.0

### 10. Peak C sound level

Number of cycle in test signal	Anticipated Value ( dB )	Measured Value, Lcpeak ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Continuous	133.0	133.0	0.0	±3.0
One	136.4	135.9	-0.5	±3.0

Number of cycle in test signal	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Continuous	133.0	133.0	0.0	±2.0
Positive half cycle	135.4	135.2	-0.2	±2.0
Negative half cycle	135.4	135.2	-0.2	±2.0

เอกสารไม่ควบคุม  
7. Kewin

# SITHIPORN ASSOCIATES CO., LTD. CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand  
Tel. +66 2433 8331 Email : calibration@sithiporn.com

SITHIPORN  
associates



Cert. No. : ACL24100  
Job No. : VC67AC0057  
Pages : 8 of 8

## 11. Overload indication

Measured value ( dB )		Deviated Value ( dB )	Acceptance Limits ( dB )
Positive one-half cycle	Negative one-half cycle		
89.7	89.7	0.0	±1.5

## 12. High level stability

Frequency Weighting	SLM Display at initial ( dB )	SLM Display at final ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor  $k = 2$   
or any value following calculation, providing a level of confidence of approximately 95 %

————— End of Calibration Certificate —————

เอกสารไม่ควบคุม  
*T. Ketchum*

## Certificate of Calibration

### Customer

Name : UNITED ANALYST AND ENGINEERING CONSULTANT CO., LTD.  
Address : 81 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Prakanong, Bangkok  
10260

Certificate No : 24-AFM-156

Request No : Req-2024-1575

### Unit Under Calibration Details

Measurement Item : Air Flow Meter  
Manufacturer : TSI Accuracy : 2% of Reading  
Model : 4146 Sensor Model : -  
Serial Number : 41462327002 Sensor Serial Number : -  
ID : UAE.EFM.125/2566 Instrument Status : Used  
Location of Calibration : LAB 4 AIR VELOCITY METER

### Calibration Environment and Details

Temperature : 23 °C ± 3 °C  
Humidity : 55 %RH ± 20 %RH  
Barometric Pressure : 1013 hPa ± 10 hPa  
Received Date : 15 July 2024  
Calibration Date : 19 August 2024  
Calibration Procedure : In-house method CP-AFM-01 by Comparison technique with Standard Primary Flow Calibrator

Reference Standard	Model	Serial Number	Traceble	Due Calibration
Air Flow Meter	Gilibrator 3 Low flow	18501010006	Sensidyne	6 August 2025
Air Flow Meter	Gilibrator 3 Standard flow	19031011003	Sensidyne	2 August 2025
Temperature meter	GT 11	08000057	Qrebom	1 March 2025
Pressure meter	CPG2400	41000KDU/651882	TPA	9 November 2024

### Traceability :

This Certificate is traceable to SI Unit through Sensidyne A2LA Accreditation No. 3943.01

### Note :

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor  $k = 2$ , providing a level of confidence approximately 95 %.

Calibration By : hne  
Mr. Noppadon Luangart  
Service Calibration Engineer

Approved By : ป.ส.ท.  
Mr. Pacit Mathavorn  
Calibration Engineer Supervisor  
Issue Date : 27 August 2024

**เอกสารไม่ควบคุม**

Certificate No : 24-AFM-156

Request No : Req-2024-1575

**Result of Calibration : Without Adjustment**

Temperature (°C)	Pressure (kPa)	STD (l/min)	UUC (l/min)	Error (l/min)	Uncertainty (l/min)	MPE (l/min)	Result
21.50	100.55	0.020	0.021	0.001	0.0013	0.005	N/A
21.30	100.53	0.050	0.052	0.002	0.0033	0.005	N/A
21.40	100.56	0.099	0.101	0.002	0.0028	0.005	N/A
21.30	100.58	0.200	0.204	0.004	0.0056	0.005	N/A
21.50	100.54	0.500	0.505	0.005	0.007	0.010	N/A
21.60	100.52	1.000	1.019	0.019	0.014	0.020	N/A
21.40	100.58	1.698	1.731	0.033	0.024	0.034	N/A
21.70	100.63	1.999	2.037	0.038	0.029	0.040	N/A
21.60	100.64	2.998	3.057	0.059	0.043	0.060	N/A
22.00	100.80	4.002	4.079	0.077	0.056	0.080	N/A
22.30	100.96	5.001	5.094	0.093	0.072	0.100	N/A

**Note**                      STD : Standard                      UUC : Unit Under Calibration  
 - UUC Reference Condition : 21.1 °C, 101.3 kPa, Air  
 - Flow Rate was corrected for non-standard operating condition by using equation :

$$Q_{meas} = Q_{ref} \times \frac{P_{ref}}{P_{meas}} \times \frac{T_{meas}}{T_{ref}}$$

where    Q = Flow Rate                      P = Absolute Pressure                      T = Absolute Temperature  
           Meas = Measurement Condition                      ref = Standard Condition

\* Indicates non accredited

MPE = Maximum Permissible Error (Specified in Manufacturer's Specifications)

N/A = Not Available, Customer does not require a statement of conformity.

**เอกสารไม่ควบคุม**



Certificate No : 24-AFM-156

Request No : Req-2024-1575

#### Decision Rule for Statements of Conformity


The standard decision rule employed for the statements of conformity to each calibration result will be applied using ILAC-G8:09/2019: Guidelines on the Reporting of Compliance with Specification as following Fig. and statements

Pass = The measurement result plus the expanded uncertainty with a 95% coverage probability were within the limit.

Pass<sup>1</sup> = The measurement result was within the limit. However, a portion of the expanded uncertainty of measurement at 95% exceeds the limit.

Fail<sup>1</sup> = The measurement result was out of the limit. However, a portion of the expanded uncertainty of measurement at 95% is within the limit.

Fail = The measurement result plus the expanded uncertainty with a 95% coverage probability were outside the limit.

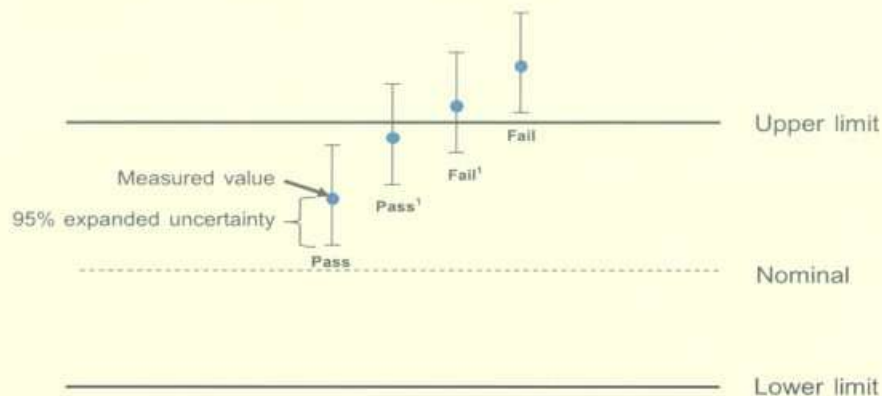

End of Certificate

เอกสารไม่ควบคุม