

ภาคผนวก ง

เอกสารสอบเทียบเครื่องมือตรวจวัด

List of Instruments Certification for Air & Noise Quality Analysis

No.	Instrument/Equipment	Parameter	Manufacturer	Model/Serial No.	Calibrator	Certification No.	Date of Calibration	Due date of Calibration	Remark
Ambient									
1	Orifice Transfer Standard Calibrator	Total Suspended Particulate (TSP) Particulate Matter < 10 µm (PM ₁₀)	Tisch Environmental, Inc.	TE-5025A 3393	Jiranatee Associates Co., Ltd.	COF-012-66	31 Aug 23	30 Aug 25	-
2	U-Tube Manometer	Total Suspended Particulate (TSP) Particulate Matter < 10 µm (PM ₁₀)	Dwyer	1221-36-W/M -	Technology Promotion Association (Thailand-Japan)	24P1252	11 Apr 24	10 Apr 25	-
3	Aneroid Barometer	Total Suspended Particulate (TSP) Particulate Matter < 10 µm (PM ₁₀)	Barigo, Germany	-	Technology Promotion Association (Thailand-Japan)	24P1367	22 Apr 24	21 Apr 25	-
4	Dial Thermo-Hygrometer	Total Suspended Particulate (TSP) Particulate Matter < 10 µm (PM ₁₀)	Barigo, Germany	-	Technology Promotion Association (Thailand-Japan)	24H752	10 Apr 24	9 Apr 25	-
5	Nitrogen Dioxide Analyzer	Nitrogen Dioxide	Thermo Scientific	42i 1201778110	UAE Consultant Co., Ltd.	17102024	17 Oct 24	16 Oct 25	-
6	Standard Gases (Mixture)	Nitrogen Dioxide	Airgas	EB0162121 2016PSIG	Airgas an Air Liquide company	E05NI91E15A0014	6 Jun 23	6 Jun 31	-
7	Sulphur Dioxide Analyzer	Sulphur Dioxide	Thermo Scientific	43i 1201778113	UAE Consultant Co., Ltd.	04092024	4 Sep 24	3 Sep 25	-
8	Standard Gases (Mixture)	Sulphur Dioxide	Airgas	EB0162121 2016PSIG	Airgas an Air Liquide company	E05NI91E15A0014	6 Jun 23	6 Jun 31	-
9	Wind Speed/Wind Direction	WS/WD	LSI Lastem	DNA202/E-LOG BQ1705627/17037708	Jiranatee Associates Co., Ltd.	CWS-027-67	7 Aug 24	6 Aug 25	-
10	Sound Level Calibrator (Acoustic Calibrator)	Calibrate Sound Level Meter	Larson Davis	CAL150 6306	Innovative Instrument Co., Ltd.	24-ACT-067	17 May 24	16 May 25	-
11	Sound Level Meter	$L_{Aeq\ 24\ hrs}$ L_{A90} L_{Amax} $L_{A_{dn}}$ ระดับเสียงรบกวน	Larson Davis	LxT1 0007305	Electrical And Electronics Institute Foundation For Industrial Development	CP20240323EA	22 Aug 24	21 Aug 25	-
12	Sound Level Meter	$L_{Aeq\ 24\ hrs}$ L_{A90} L_{Amax} $L_{A_{dn}}$ ระดับเสียงรบกวน	Larson Davis	LxT1 0007306	Electrical And Electronics Institute Foundation For Industrial Development	CP20240290EA	5 Aug 24	4 Aug 25	-

List of Instruments Certification for Air & Noise Quality Analysis

No.	Instrument/Equipment	Parameter	Manufacturer	Model/Serial No.	Calibrator	Certification No.	Date of Calibration	Due date of Calibration	Remark
Stack									
1	Pre-Test Console	Total Suspended Particulate	Apex Instruments, USA.	XC-572-V 1904011	Envi Equipment Service Co., Ltd.	E24-080073	21 Aug 24	20 Aug 25	-
2	Flue gas Analyzer	Sulphur Dioxide Oxide of Nitrogen as Nitrogen Dioxide Carbon Monoxide Oxygen	Testo	Testo 350 60899698/701	Entech Industrial Sulation Co., Ltd.	G 670083	8 Feb 24	7 Feb 25	-

List of Instruments Certification for Air & Noise Quality Analysis

No.	Instrument/Equipment	Parameter	Manufacturer	Model/Serial No.	Calibrator	Certification No.	Date of Calibration	Due date of Calibration	Remark
Workplace									
1	Sound Level Calibrator (Acoustic Calibrator)	Calibrate Sound Level Meter	Larson Davis	CAL150 6306	Innovative Instrument Co.,Ltd.	24-ACT-067	17 May 24	16 May 25	-
2	Sound Level Meter	$L_{Aeq\ 8\ hrs}$, L_{Amax}	Rion, Japan	NL-42 00408982	Sithiporn Associates Co., Ltd.	ACL24051	18 Jan 24	17 Jan 25	-
3	Sound Level Meter	$L_{Aeq\ 8\ hrs}$, L_{Amax}	Rion, Japan	NL-42 00709655	Sithiporn Associates Co., Ltd.	ACL24060	18 Jan 24	17 Jan 25	-
4	Sound Level Meter	$L_{Aeq\ 8\ hrs}$, L_{Amax}	Rion, Japan	NL-42 00409023	Sithiporn Associates Co., Ltd.	ACL24160	4 Jun 24	3 Jun 25	-
5	Thermal Environment Monitor	Heat Meter	Quest Technologies, Inc	QuesTemp 34 TEG100075	Innovative Instrument Co.,Ltd.	24-TPM-047	23 Jan 24	22 Jan 25	-
6	Thermal Environment Monitor	Heat Meter	3M	QuesTemp 32 TPQ020025	Innovative Instrument Co.,Ltd.	24-TPM-152	21 Mar 24	20 Mar 25	-
7	Thermal Environment Monitor	Heat Meter	TSI QUEST	QuesTemp 32 TPT060013	Innovative Instrument Co.,Ltd.	24-TPM-043	23 Jan 24	22 Jan 25	-
8	Digital Lux Meter	Lux	Extech Instrument, Taiwan	407026 A 052267	Innovative Instrument Co., Ltd.	24-LXM-051	29 Feb 24	28 Feb 25	-



JIRANATEE ASSOCIATES CO.,LTD.

Jiranatee Associates Co.,Ltd
63/14-15, 67/35-36
Petchkasem 7,7/1, Rd. Watthapra, Bangkokyai,
Bangkok 10600 (Thailand)
Tel: +6608680812
Mobile: +66863999453
E-mail: jnac-calibration@jiranatee.com
Web site: www.jiranatee.com

Accredited calibration laboratory
ISO/IEC 17025:2017
NSC-TISI-TIS 17025
CALIBRATION 0367

Flow measurement laboratory
Calibration services department.



CERTIFICATE OF CALIBRATION

Certificate No. : COF-012-66

Page 1 of 2 Pages

MEASUREMENT ITEM : Top Load Orifice
MANUFACTURER : TISCH
MODEL/TYPE : TE-5025A
SERIAL NUMBER : 3393
ID NUMBER : UAE.EFM.064/2560
CONDITION AS-RECEIVED : Used item
CUSTOMER : United Analyst and Engineering Consultant Co., Ltd.
81 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong,
Bangkok 10260

RECEIVED DATE : 14 Aug 2023
MEASUREMENT DATE : 31 Aug 2023
ISSUE DATE : 01 Sep 2023

ENVIRONMENTAL CONDITIONS:

Ambient condition in the laboratory are as follow:

Temperature	: 23.0 ± 3.0	°C
Relative Humidity	: 55.0 ± 15.0	%RH
Atmospheric Pressure	: 1010 ± 10	hPa

CALIBRATION CONDITION:

Preconditioning : 24 hours at ambient conditions.
Measurement Condition : The average values during measurement are 23.8 °C and 56.3 %RH.

NOTED: The certificate is valid only to the item calibrated on date and place of calibration.

TABULATION OF RESULTS:

The table on next page give the measured values.

Calibration procedure:

The Orifice gas flow device was calibrated against Standard Rotary Displacement Meter (Roots Meter) Model G65/IMC/W2-dp. The WI-CL-004 was used as a calibration guideline.

Traceability:

This certificate provides a traceability of The measurement to recognized the national standards, and to realization of the international system of units (SI) through the VSL (National Metrology Institute of Netherlands) via Certificate number: G2211901

Uncertainty of Measurement:


The reported uncertainty of measurement is based on the standard uncertainty multiplied by a coverage factor $k=2$, Which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty has been determined in accordance with the GUM 'Evaluation of measurement data - Guide to the expression of uncertainty in measurement'

Calibrated by:

- ☐ Mr. Sorawit Thachalad
☒ Miss Jitraporn Lertsomphol



Approved signatory:

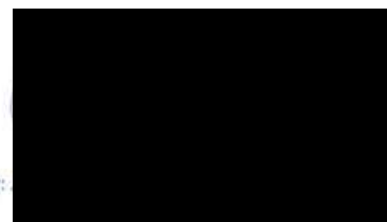

Calibration Department Manager

เอกสารไม่ควบคุม

MEASUREMENT RESULTS:

The Orifice gas flow device was calibrated by direct comparison method with the Standard Rotary Displacement Meter (Roots Meter). The Humid air was used as a medium in the system. The standard conditions are 25°C (298.15 K) and 760 mmHg for standard temperature and standard pressure respectively.

Table 1: The results of Q Standard calibration data

Plate	Flow rate m^3/min	Pressure [Pa] mmHg	Temperature [Ta] °C	Temperature [Tm] °C	Δp_{meter} mmHg	$\Delta p_{Orifice}$ inH ₂ O	Y	Standard Flow [Q_s] m^3/min
1	0.694	754.292	24.08	23.49	55.071	1.682	1.294	0.642
2	1.000	754.269	24.02	23.63	60.844	3.423	1.846	0.916
3	1.122	754.201	23.85	23.51	42.018	4.559	2.131	1.056
4	1.169	754.302	23.77	23.43	30.532	5.122	2.259	1.119
5	1.409	754.198	23.89	23.66	29.917	7.496	2.733	1.349

Slope (m): 2.03291
 Intercept (b): -0.01401
 Correlation coefficient (r): 0.99983
 Uncertainty ($k=2$): 0.015 m^3/min

Table 2: The results of Q actual calibration data

Plate	Flow rate m^3/min	Pressure [Pa] mmHg	Temperature [Ta] °C	Temperature [Tm] °C	Δp_{meter} mmHg	$\Delta p_{Orifice}$ inH ₂ O	Y	Standard Flow [Q_s] m^3/min
1	0.694	754.292	24.08	23.49	55.071	1.682	0.814	0.645
2	1.000	754.269	24.02	23.63	60.844	3.423	1.161	0.920
3	1.122	754.201	23.85	23.51	42.018	4.559	1.340	1.060
4	1.169	754.302	23.77	23.43	30.532	5.122	1.420	1.123
5	1.409	754.198	23.89	23.66	29.917	7.496	1.718	1.354

Slope (m): 1.27329
 Intercept (b): -0.00881
 Correlation coefficient (r): 0.99983
 Uncertainty ($k = 2$): 0.015 m^3/min

End of Certificate of Calibration



เอกสารไม่ควบคุม



Certificate of Calibration

Certificate No. : 24P1252

Page : 1 of 2

Equipment : U Tube Manometer

Manufacturer: Dwyer

Model : 1221-36-W/M

Serial No.: -

ID No.: UAE.EFM.078/2566

Condition As-Received: Used Item

Received Date: 03 April 2024

Calibration Date: 11 April 2024

Reference: 2404-0118WSC

Ambient Temperature: (23 ± 2) °C

Relative Humidity: (50 ± 15) %

Atmospheric Pressure: 1011 mbar

Submitted by: United Analyst and Engineering Consultant Co.,Ltd.

This certificate may not be reproduced other than in full,
except with the prior written approval of the head of
Corporate Services 3: Equipment Calibration and Testing Services.

81 Soi Udomsuk 41, Sukhumvit Road, Bangchak,
Phrakhanong, Bangkok 10260

Procedure used: The calibration was conducted by direct comparison method against Pressure Measuring Instruments Standard according to calibration procedure CP-P04, using " DKD-R 6-1 ; Calibration of Pressure Gauges " as a guidelines.

Condition of this result of calibration

1.Reference standards instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Certificate No.</u>	<u>Due Date</u>
1) Pressure Calibrator	PC106P	1189	MP-0176-23	12 Sep 2024

2.This result of calibration was made on requested at the point specified by customer.

3.Scale and conversion factor is 1 kPa = 4.0146293 inH₂O

4.This instrument was used clean air as pressure media.

5.This instrument was calibrated by applied pressure to high-port (+) side and low-port (-) side open to atmospheric pressure.

6.This instrument was installed in vertical orientation and top of the pressure port was used as the reference level.

7.The certificate is valid only to the item calibrated on date and place of calibration.


8.This Certification is traceable to the International System of Unit maintained through:-

-National Institute of Metrology (Thailand), NSC-ONSC Accredited No. Calibration 0144

Calibrated by : Suksan Khankaew

Issue Date : 17 April 2024

Approved Signatory :



เอกสารไม่ควบคุม



Cert.No.: 24P1252

Page: 2 of 2

Result of calibration:- Without adjustment

Range : 0 inH₂O to 36 inH₂O

Function:- Pressure Measurement

Scale Interval : 0.1 inH₂O (The Second Estimate)

Increasing Pressure

<u>Applied Pressure</u>	<u>High-port side</u>	<u>UUC Indication</u>		<u>ΔP</u>	<u>Error</u>
		<u>Low-port side</u>			
0.00	0.00	0.00		0.00	0.00
2.00	1.00	-1.00		2.00	0.00
4.00	2.00	-2.00		4.00	0.00
6.00	3.00	-3.00		6.00	0.00
8.00	4.00	-4.00		8.00	0.00
10.00	5.00	-5.00		10.00	0.00
12.00	6.00	-6.00		12.00	0.00
14.00	7.00	-7.05		14.05	0.05
16.00	8.00	-8.05		16.05	0.05
18.00	9.00	-9.05		18.05	0.05
20.00	10.00	-10.10		20.10	0.10
22.00	11.00	-11.10		22.10	0.10
24.00	12.00	-12.10		24.10	0.10
26.00	13.00	-13.10		26.10	0.10
28.00	14.00	-14.10		28.10	0.10
30.00	15.00	-15.10		30.10	0.10
32.00	16.00	-16.10		32.10	0.10
34.00	17.05	-17.10		34.15	0.15
35.80	18.00	-18.00		36.00	0.20

The uncertainty of measurement was ± 0.11 inH₂O

* ΔP = High-port side - Low-port side

* UUC = Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95 %.

-oOo-

เอกสารไม่ควบคุม



Certificate of Calibration

Certificate No. : 24P1367

Page : 1 of 2

Equipment : Aneroid Barometer

Manufacturer: Barigo

Model : -

Serial No.: -

ID No.: UAE.ANV.152/2550

Condition As-Received: Used Item

Received Date: 05 April 2024

Calibration Date: 22 April 2024

Reference: 2404-0243WSC

Ambient Temperature: (23 ± 2) °C

Relative Humidity: (50 ± 15) %

Atmospheric Pressure: 1007 mbar

Submitted by: United Analyst and Engineering Consultant Co.,Ltd.

81 Soi Udomsuk 41, Sukhumvit Road, Bangchak,
Phrakhanong, Bangkok 10260

Procedure used: The calibration was conducted by direct comparison method against Pressure Measuring Instruments Standard according to calibration procedure CP-P10, using " DKD-R 6-1 ; Calibration of Pressure Gauges " as a guidelines.

Condition of this result of calibration

1.Reference standards instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Certificate No.</u>	<u>Due Date</u>
1) Standard Barometer	DPI142	1422505046	MP-0094-23	03 May 2024

2.This instrument was installed in vertical orientation and center of the dial was used as the reference level.

3.This result of calibration was made on requested at the point specified by customer.

4.This result of calibration instrument was in absolute pressure.

5.This instrument was used clean air as pressure media.

6.The certificate is valid only to the item calibrated on date and place of calibration.


7.This Certification is traceable to the International System of Unit maintained through:-

-National Institute of Metrology Thailand (NIMT)

Calibrated by : Suksan Khankaew

Issue Date : 23 April 2024

Approved Signatory :

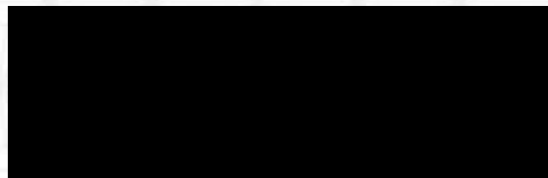

เอกสารไม่ควบคุม



Cert.No.: 24P1367

Page: 2 of 2

Result of calibration:- Without adjustment

Range : 960 hPa to 1030 hPa

Function:- Absolute Pressure Measurement

Scale Interval : 1 hPa (The Fifth Estimate)

Increasing Pressure

Applied Pressure (hPa)	957.13	968.77	980.13	990.56	1001.26	1011.35	1022.10	1032.61
UUC* Indication (hPa)	960.0	970.0	980.0	990.0	1000.0	1010.0	1020.0	1030.0
Error (hPa)	2.87	1.23	-0.13	-0.56	-1.26	-1.35	-2.10	-2.61

Decreasing Pressure

Applied Pressure (hPa)	1032.61	1021.84	1010.88	1000.82	990.20	979.52	968.48	957.17
UUC* Indication (hPa)	1030.0	1020.0	1010.0	1000.0	990.0	980.0	970.0	960.0
Error (hPa)	-2.61	-1.84	-0.88	-0.82	-0.20	0.48	1.52	2.83

The uncertainty of measurement was ± 0.25 hPa

* UUC = Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95 %.

-oOo-

เอกสารไม่ควบคุม



Certificate of Calibration

Certificate No. : 24H752

Page : 1 of 2

Equipment : Dial Thermo-Hygrometer

Manufacturer: Barigo

Model : -

Serial No.: -

ID No.: UAE.ANV.004/2548

Condition As-Received: Used Item

Received Date: 05 April 2024

Calibration Date: 10 April 2024
to 18 April 2024

Reference: 2404-0247WSC

Ambient Temperature: (25 \pm 3) °C

Relative Humidity: (50 \pm 20) %

This certificate may not be reproduced other than in full,
except with the prior written approval of the head of
Corporate Services 3: Equipment Calibration and Testing Services.

Submitted by: United Analyst and Engineering Consultant Co.,Ltd.

81 Soi Udomsuk 41, Sukhumvit Road,
Bangchak, Phrakhanong, Bangkok 10260

Procedure used: Calibration were conducted using in-house calibration procedure CP-H02 according to comparison
with standard chilled mirror sensor for humidity measurement function and comparison with standard
temperature probe for temperature measurement function into humidity / temperature chamber.

Condition of this result of calibration

1.Reference standards instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Certificate No.</u>	<u>Due Date</u>
1) Chilled Mirror Hygrometer	Dew Master	44730	21656	02 Aug 2024
2) Handheld Thermometer With Sensor	1521	A5A339	2311238	16 Oct 2024

2.The certificate is valid only to the item calibrated on date and place of calibration.

3.This Certification is traceable to the International System of Unit maintained through:-

-Thunder Scientific Corporation, NVLAB Accreditation No. Calibration 200582-0

-Technology Promotion Association (Thailand-Japan), NSC-ONSC Accredited No. Calibration 0008

Calibrated by : Chakrit Waewwanjua
Issue Date : 18 April 2024

Approved Signatory :



เอกสารไม่ควบคุม



Cert. No.: 24H752

Page.: 2 of 2

Result of Calibration:-

Without Adjustment

Function:

Humidity Measurement.

<u>Reference Temperature</u> (°C)	<u>Standard Humidity</u> (%R.H.)	<u>UUC* Reading</u> (%R.H.)	<u>Error</u> (%R.H.)	<u>Uncertainty of Measurement</u> (±%R.H.)
25.0	40.1	41	0.9	1.6
25.0	60.0	60	0.0	1.7
25.0	80.0	78	-2.0	1.8

Result of Calibration:-

Without Adjustment

Function:

Temperature Measurement.

<u>Standard Temperature</u> (°C)	<u>UUC* Reading</u> (°C)	<u>Error</u> (°C)	<u>Uncertainty of Measurement</u> (±°C)
20.014	20.5	0.486	0.72
25.033	25.0	-0.033	0.72
30.010	30.0	-0.010	0.72
35.027	34.5	-0.527	0.72
40.013	39.5	-0.513	0.72

UUC* : Unit Under Calibration

The reported uncertainty of measurement was base on standard uncertainty multiplied by coverage factor $k = 2.00$, providing confidence level approximately 95%.

-o0o-

เอกสารไม่ควบคุม

MULTI-POINT GAS TEST REPORT

Test Date : Oct 17, 2024

Equipment : Gas Analyzer (NO₂)

Model : 42i

Manufacturer : Thermo Scientific

Serial Number : 1201778110

Standard Gas Concentration


Sulphur Dioxide (SO ₂)	42.89
Nitric Oxide (NO)	46.77
Methane (CH ₄)	-
Carbon Monoxide (CO)	965.9
Cylinder No. :	EB0159156
Expiration Date :	Nov 6, 2026

Dilutor Detail

Manufacturer :	Thermo Scientific
Model :	146i
Serial Number :	1180540071

Multi-point gas test data

Reference Value (ppb)			Analyzer Display (ppb)	Difference Error	Percent Error	[% Error]
Level 1	Zero	0.0	0.0	0.00	0.00	0.00
Level 2	20.00%	100.0	100.6	0.60	0.60	0.60
Level 3	40.00%	200.0	200.9	0.90	0.45	0.45
Level 4	60.00%	300.0	300.5	0.50	0.17	0.17
Level 5	80.00%	400.0	400.0	0.00	0.00	0.00
Remark : Measuring Range 500.0 ppb				Average Difference (%)		0.24

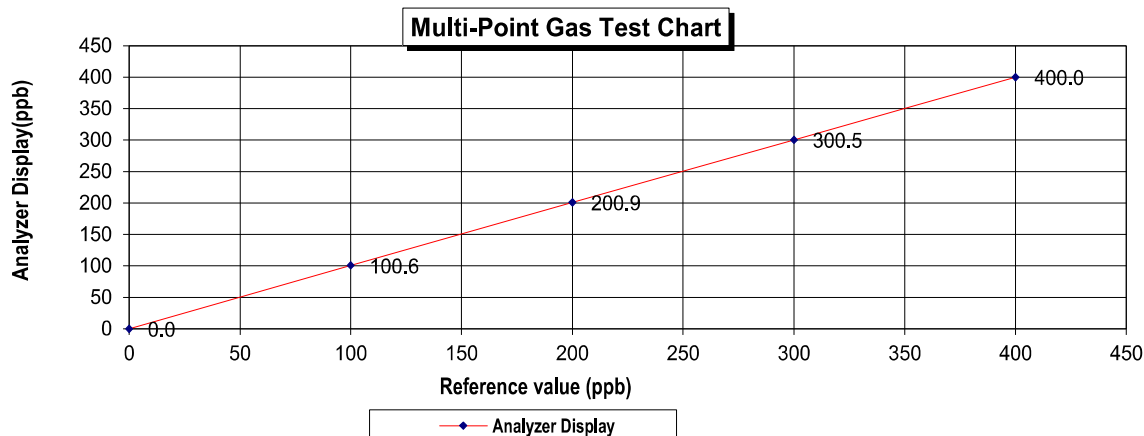

17 / 10 / 2567
...../...../.....



17 Oct 2024
...../...../.....

CERTIFICATE OF ANALYSIS

Grade of Product: EPA PROTOCOL STANDARD

Customer: AIR LIQUIDE (THAILAND)

LTD--

Part Number: E05N191E15A0014

Cylinder Number: EB0162121

Laboratory: 124 - Plumsteadville - PA

PGVP Number: A12023

Gas Code: CO,CO2,NO,NOX,SO2,BALN

Reference Number: 160-402772205-1

Cylinder Volume: 144.0 CF

Cylinder Pressure: 2016 PSIG

Valve Outlet: 660

Certification Date: Jul 06, 2023

Expiration Date: Jul 06, 2031

Certification performed in accordance with "EPA Traceability Protocol for Assay and Certification of Gaseous Calibration Standards" (May 2012) document EPA 800/R-12/531, using the assay procedures listed. Analytical Methodology does not require correction for analytical interference. This cylinder has a total analytical uncertainty as stated below with a confidence level of 95%. There are no significant impurities which affect the use of this calibration mixture. All concentrations are on a mole/mole basis unless otherwise noted. The results relate only to the items tested. The report shall not be reproduced except in full without approval of the laboratory. Do Not Use This Cylinder below 100 psig, i.e. 0.7 megapascals.

ANALYTICAL RESULTS

Component	Requested Concentration	Actual Concentration	Protocol Method	Total Relative Uncertainty	Assay Dates
NOX	100.0 PPM	100.4 PPM	G1	+/- 0.9% NIST Traceable	06/27/2023, 07/06/2023
NITRIC OXIDE	100.0 PPM	100.2 PPM	G1	+/- 0.9% NIST Traceable	06/27/2023, 07/06/2023
SULFUR DIOXIDE	100.0 PPM	100.0 PPM	G1	+/- 1.4% NIST Traceable	06/27/2023, 07/06/2023
CARBON MONOXIDE	200.0 PPM	199.2 PPM	G1	+/- 0.3% NIST Traceable	06/26/2023
CARBON DIOXIDE	8.000 %	7.982 %	G1	+/- 1.2% NIST Traceable	06/27/2023
NITROGEN	Balance				

CALIBRATION STANDARDS

Type	Lot ID	Cylinder No	Concentration	Uncertainty	Expiration Date
GMIS	104202308	CC754364	98.36 PPM NITRIC OXIDE/NITROGEN	+/- 0.4%	Jan 04, 2031
PRM	C2219101	APE1514048	100.19 PPM NITRIC OXIDE/NITROGEN	+/- 0.3%	Feb 28, 2025
GMIS	2023042525	CC754381	98.52 PPM NITRIC OXIDE/NITROGEN	+/- 0.4%	Apr 25, 2031
PRM	12409	D913660	15.01 PPM NITROGEN DIOXIDE/AIR	+/- 1.5%	Feb 17, 2023
GMIS	153400202002	EB0130037	9.693 PPM NITROGEN DIOXIDE/NITROGEN	+/- 1.6%	Sep 29, 2025
NTRM	160102-22	KAL003820	97.69 PPM SULFUR DIOXIDE/NITROGEN	+/- 0.8%	Nov 01, 2027
CO	230601	CC745902	249.47 PPM CARBON MONOXIDE/NITROGEN	+/- 0.3%	Dec 09, 2028
NTRM	130606-02	CC411730	13.359 % CARBON DIOXIDE/NITROGEN	+/- 0.6%	May 14, 2025

The SRM, NTRM, PRM, or RGM noted above is only in reference to the GMIS used in the assay and not part of the analysis.

ANALYTICAL EQUIPMENT

Instrument/Make/Model	Analytical Principle	Last Multipoint Calibration
Nicolet iS50 FTIR AUP2010245 CO2	FTIR	Jun 15, 2023
SIEMENS ULTRAMAT6E N1-C8-180	NDIR	Jun 14, 2023
Nicolet iS50 FTIR AUP2010245 NO	FTIR	Jun 29, 2023
Nicolet iS50 FTIR AUP2010245 NO2	FTIR	Jun 15, 2023
Nicolet iS50 FTIR AUP2010245 SO2	FTIR	Jun 08, 2023

Approved for Release

Page 1 of 1

เอกสารไม่ควบคุม

MULTI-POINT GAS TEST REPORT

Test Date : Sep 4, 2024

Equipment : Gas Analyzer (SO₂)

Model : 43i

Manufacturer : Thermo SCIENTIFIC

Serial Number : 1201778113

Standard Gas Concentration

Sulphur Dioxide (SO ₂)	42.89
Nitric Oxide (NO)	46.77
Methane (CH ₄)	-
Carbon Monoxide (CO)	965.9
Cylinder No. :	EB0159156
Expiration Date :	Nov 06, 2026


Dilutor Detail

Manufacturer :	Thermo SCIENTIFIC
Model :	146i
Serial Number :	1180540071

Multi-point gas test data

	Reference Value (ppb)		Analyzer Display (ppb)	Difference Error	Percent Error	[% Error]
Level 1	Zero	0.0	0.0	0.00	0.00	0.00
Level 2	20.00%	100.0	100.3	0.30	0.30	0.30
Level 3	40.00%	200.0	200.9	0.90	0.45	0.45
Level 4	60.00%	300.0	300.7	0.70	0.23	0.23
Level 5	80.00%	400.0	400.0	0.00	0.00	0.00
Remark : Measuring Range			500.0 ppb	Average Difference (%)		0.20
:Acceptable Limit $\pm 5\%$						

Multi-Point Gas Test Chart

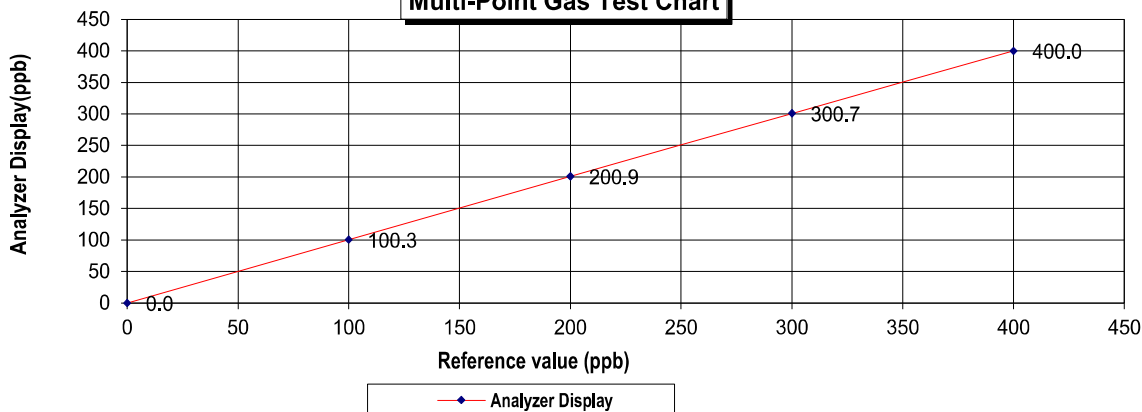

4 / 9 / 2567

4 / Sep / 2024



JIRANATEE ASSOCIATES CO., LTD.

Jiranatee Associates Co., Ltd.
63/14-15, 67/35-36
Petchkasem 7,7/1, Rd. Watthapra, Bangkokyal,
Bangkok 10600 (Thailand)
Tel: +6608680812
Mobile: +66863999453
E-mail: jnac-calibration@jiranatee.com
Web site: www.jiranatee.com

Accredited calibration laboratory
ISO/IEC 17025:2017
NSC-TISI-TIS 17025
CALIBRATION 0367

Air speed measurement laboratory
Calibration services department.



Certificate Number

CWS-027-67

CERTIFICATE OF CALIBRATION

Page 1 of 2 Pages

MEASUREMENT ITEM : Cup anemometer
MANUFACTURER : LSI Lastem
MODEL/TYPE : Sensor: DNA202
Data logger: E-LOG
SERIAL NUMBER : Sensor: BQ1705627
Data logger: 17037708
ID NUMBER : -
CONDITION AS-RECEIVED : Used item
CUSTOMER : United Analyst and Engineering Consultant Co., Ltd.
81 Soi Udomsuk 41, Sukhumvit Road, Bangchak,
Phrakhanong, Bangkok 10260

RECEIVED DATE : 02 Aug 2024
MEASUREMENT DATE : 07 Aug 2024
ISSUE DATE : 09 Aug 2024

ENVIRONMENTAL CONDITIONS:

Ambient condition in the laboratory are as follow:

Temperature : 23.0 ± 3.0 °C
Relative Humidity : 55.0 ± 15.0 %RH
Atmospheric Pressure : 1010 ± 10 hPa

PLACE OF CALIBRATION : Eiffel-type wind tunnel of Jiranatee Associates Co., Ltd.

CALIBRATION CONDITIONS : Wind tunnel cross-section area¹ 900 cm²
Wind direction frontal area² 195 cm²
Diameter of mounting pipe³ - mm
Blockage ratio of test object⁴ 0.217 [-]

Preconditioning : 24 hours at ambient conditions.

Measurement Condition : The average values during measurement are (23.8) °C, (41.5) %RH and (1009.0) hPa.

TABULATION OF RESULTS:

The table on next page give the measured values.

Calibrated by:

☒ Mr. Sorawit Thachalad
☐ Miss Jittraporn Lertsomphol



Approved signatory:

Calibration Department Manager

Remark:

¹ Nozzle cross-section area of the wind tunnel

² Projected cross-section area of the tested object include mounting pipe

³ Diameter of mounting pipe

⁴ Ratio ² to ¹

Calibration procedure:

The Cup anemometer was calibrated against Standard air velocity transducer model: 8455-12 and pitot tube with precision differential pressure meter model: DPM2500 in an close test-section of Eiffel-type wind tunnel with 900 cm² cross test section area. The WI-CL-007 based on IEC 61400-12-1, Wind energy generation systems – Part 12-1: Power performance measurements of electricity producing wind turbines, March 2017 was used as a calibration guideline.

Traceability:

This certificate provides a traceability of The measurement to recognized the national standards, and to realization of the international system of units (SI) through the NIMT (National Metrology Institute of Thailand) via Certificate number: MW-0007-24 and MW-0055-23.

Uncertainty of Measurement:

The reported uncertainty of measurement is based on the standard uncertainty multiplied by a coverage factor $k=2$, Which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty has been determined in accordance with the GUM 'Evaluation of measurement data - Guide to the expression of uncertainty in measurement'

MEASUREMENT RESULTS ⁵

The Cup anemometer, Unit Under Calibration (UUC) was exercised at 10 m/s for 5 minutes prior to calibration being performed. The standard air velocity 0.5 m/s to 5 m/s was calculated by a standard air velocity transducer which was installed 50 mm away from wind tunnel nozzle and installed 40 mm away from top of the test section and the standard air velocity 5 m/s to 30 m/s was calculated by a pitot tube with precision differential pressure meter which was installed 50 mm away from wind tunnel nozzle and installed 40 mm away from top of the test section, UUC was mounted on a round vertical tube of the lower plate at center of test section. The calibration was carried out under both rising and falling air velocity in the range of 1 m/s to 16 m/s at calibration interval of 1 m/s. The results of calibration and associated measurement uncertainties are reported in the table below.

V_{std} (m/s)	Temp. wind tunnel (°C)	Temp. room (°C)	V_{UUC} (m/s)	Error (m/s)	$U (k=2)$ (m/s)
1.093	23.98	24.05	0.9	-0.2	0.31
2.051	24.24	24.05	1.8	-0.3	0.31
3.124	24.02	24.05	2.9	-0.2	0.31
4.086	24.04	24.05	3.8	-0.3	0.31
5.09	23.68	24.05	4.9	-0.2	0.31
6.08	23.84	24.05	5.9	-0.2	0.31
6.99	23.52	24.05	6.8	-0.2	0.31
8.16	24.48	24.05	8.0	-0.2	0.31
9.12	23.50	24.05	9.1	-0.1	0.31
9.98	24.02	24.05	9.9	-0.1	0.31
11.04	23.46	24.05	11.1	0.0	0.31
12.05	23.64	24.05	12.1	0.1	0.31
13.02	23.46	24.05	13.0	-0.1	0.31
13.96	23.50	24.05	14.0	0.1	0.35
15.03	23.52	24.05	15.1	0.1	0.39
16.00	23.50	24.05	16.0	0.0	0.34

Remark:

⁵ Calibration results only count for the tested circumstances and environmental conditions during which calibration took place

⁶ Velocity of standard

⁷ Velocity of Unit Under Calibration

PHOTO OF CALIBRATION SET-UP



Calibration set-up of the Cup anemometer calibration in the wind tunnel of Jiranatee Associates Co., Ltd. The Cup anemometer shown may differ from the calibrated one. Remark: The proportion of the set-up is not true to scale due to imaging geometry.



เอกสารไม่ควบคุม



JIRANATEE ASSOCIATES CO.,LTD.

Jiranatee Associates Co.,Ltd
63/14-15, 67/35-36
Petchkasem 7,7/1, Rd. Watthapra, Bangkokyal,
Bangkok 10600 (Thailand)
Tel: +6608680812
Mobile: +66863999453
E-mail: jnac-calibration@jiranatee.com
Web site: www.jiranatee.com

Accredited calibration laboratory
ISO/IEC 17025:2017
NSC-TISI-TIS 17025
CALIBRATION 0367

Wind direction measurement laboratory
Calibration services department.



NSC – TISI – TIS 17025
CALIBRATION 0367

Certificate Number

CWD-027-67

CERTIFICATE OF CALIBRATION

Page 1 of 2 Pages

MEASUREMENT ITEM : Wind Direction Sensor
MANUFACTURER : LSI Lastem
MODEL/TYPE : Sensor: DNA212
Data logger: E-LOG
SERIAL NUMBER : Sensor: 19020250
Data logger: 17037708
ID NUMBER : -
CONDITION AS-RECEIVED : Used item
CUSTOMER : United Analyst and Engineering Consultant Co., Ltd.
81 Soi Udomsuk 41, Sukhumvit Road, Bangchak,
Phrakhanong, Bangkok 10260

RECEIVED DATE : 02 Aug 2024
MEASUREMENT DATE : 08 Aug 2024
ISSUE DATE : 09 Aug 2024

ENVIRONMENTAL CONDITIONS:

Ambient condition in the laboratory are as follow:

Temperature : 23.0 ± 3.0 °C
Relative Humidity : 55.0 ± 15.0 %RH
Atmospheric Pressure : 1010 ± 10 hPa

PLACE OF CALIBRATION : Eiffel-type wind tunnel of Jiranatee Associates Co., Ltd.

CALIBRATION CONDITION : Wind tunnel cross-section area¹ 900 cm²
Wind direction frontal area² 52 cm²
Diameter of mounting pipe³ - mm
Blockage ratio of test object⁴ 0.058 [-]

Preconditioning : 24 hours at ambient conditions.

Measurement Condition : The average values during measurement are (24.9)°C, (45.1) %RH and (1005.2) hPa.

TABULATION OF RESULTS:

The table on next page give the measured values.

Calibrated by:

- ☒ Mr. Sorawit Thachalad
☐ Miss Jittrapoln Lertsomphol



Approved signatory: ..



Calibration Department Manager

Remark:

- ¹ Nozzle cross-section area of the wind tunnel
² Projected cross-section area of the tested object include mounting pipe
³ Diameter of mounting pipe
⁴ Ratio ² to ¹

MEASUREMENT RESULTS⁵

The wind direction sensor was calibrated against standard rotary encoder by comparison method. During calibration, the measurement was carried out at 45° intervals in clockwise and counterclockwise directions after offset adjustment has been made. The flow speed of wind tunnel (usually 5 m/s) is kept constant while the sensor is rotated around its vertical axis. The results of calibration and associated measurement uncertainties are reported in the table below.

Air speed m/s	D°_{std} Degree (°)	D°_{unc} Degree (°)	Error Degree (°)	$U (k=2)$ Degree (°)
5.01	0.000	0	0	0.80
	45.000	46	1	0.80
	90.000	90	0	0.80
	135.000	135	0	0.80
	180.000	180	0	0.80
	225.000	225	0	0.80
	270.000	269	-1	0.80
	315.000	314	-1	0.80

Remark:

⁵ Calibration results only count for the tested circumstances and environmental conditions during which calibration took place

⁶ Direction of standard

⁷ Direction of Unit Under Calibration

End of Certificate of Calibration



เอกสารไม่ควบคุม

Certificate of Calibration

Customer

Name : UNITED ANALYST AND ENGINEERING
CONSULTANT CO.,LTD.
Address : 81 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Prakanong,
Bangkok 10260

Certificate No : 24-ACT-067
Request No : Req-2024-1024

Unit Under Calibration Details

Measurement item : Acoustic Calibrator Class : 2
Manufacturer : LARSON DAVIS Range : 94 , 114 dB / 1000 Hz
Model : CAL150 Instrument Status : Used
Serial Number : 6306
ID : UAE.EFM.048/2563

Calibration Environment and Details

Temperature : (23 ±2 °C)
Humidity : (50 ± 20 %RH)
Barometric Pressure : (1013 ±10.0 hPa)
Received Date : 8 May 2024
Calibration Date : 17 May 2024
Location of Calibration : LAB 1 Acoustic
Calibration Procedure : In-house method CP-ACT-02 based on IEC 60942:2017 Electroacoustics - Sound calibrators

Reference Standard	Model	Serial Number	Traceable	Due Calibration
Sound Calibrator	SV 35A	58079	EEI	31 May 2024
THD Multimeter	2015	1047765	NIMT	16 January 2025

Traceability : This certificate provides traceability of measurement to recognized national standard, and to the realization of the international System of Units (SI).

Note

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor k=2, providing a level of confidence approximately 95 %.

Calibrated By :



Service Calibration Engineer

Approved By :



Calibration Engineer Supervisor

Issue Date : 17 May 2024

Certificate No : 24-ACT-067

Request No : Req-2024-1024

Sound pressure level

Calibration Results : Without Adjustment

Calibration Range (dB)	Without Adjustment (dB)		Adjustment (dB)		Uncertainty (\pm dB)	Acceptance limit Class 2 (\pm dB)
	Measured	Deviated value	Measured	Deviated value		
94 dB / 1000 Hz	94.09	0.09	-	-	0.13	0.40
114 dB / 1000 Hz	114.10	0.10	-	-	0.13	0.40

Frequency of Sound pressure level

Calibration Range (Hz)	Without Adjustment		Adjustment		Uncertainty (\pm %)	Acceptance limit Class 2 (\pm %)
	Measured (Hz)	Deviated value	Measured (Hz)	Deviated value		
94 dB / 1000 Hz	1000.00	0.00	-	-	0.01	1.7
114 dB / 1000 Hz	1000.00	0.00	-	-	0.01	1.7

Total Harmonic Distortion plus Noise of Sound pressure level (THD+N %)

Calibration Range (Hz)	Without Adjustment	Adjustment	Uncertainty (\pm %)	Acceptance limit Class 2 (\pm %)
	Measured (%)	Measured (%)		
94 dB / 1000 Hz	0.05	-	0.40	3.0
114 dB / 1000 Hz	0.21	-	0.40	3.0

Note :

Function	Maximum-permitted Uncertainty of measurement
Sound pressure level	0.35 dB
Frequency	0.20%
Total distortion+noise	1.00%

- Acceptance limit was IEC60942:2017 Class 1

- The calibration results exclude the calibrator pressure correction

- The calibration results exclude the microphone volume correction

End of Calibration



**ELECTRICAL AND ELECTRONICS INSTITUTE
FOUNDATION FOR INDUSTRIAL DEVELOPMENT**

975 Moo 4, Bangpoo Industrial Estate, Soi 8, Sukhumvit Road km 37,

Phraek Sa, Mueang Samut Prakan, Samut Prakan 10280

Tel: +66 2709 4860 Fax: +66 2324 0917



Certificate No.: CP20240323EA

Operation No.: CP2024080294

Certificate of Calibration

Equipment: Sound Level Meter

Manufacturer: Larson Davis (Meter), PCB (Microphone), PCB (Preamplifier)

Model/Type: LxT1 (Meter), 377B02 (Microphone), PRMLxT1 (Preamplifier)

Serial No.: 0007305 (Meter), 345234 (Microphone), 077640 (Preamplifier)

ID No.: UAE.EFM.038/2566

Customer: United Analyst and Engineering Consultant Co.,Ltd.

Address: 81 Soi Udomsuk 41, Sukhumvit Road, Bangchak
Phrakhanong, Bangkok 10260


Received Date: 9 August 2024

Calibrated Date: 22 - 27 August 2024

Issued Date: 28 August 2024

Calibrated by: Ms. Juntaporn Kunhakom

Approved by: _____



Group Manager

This report was prepared electronically using applicable electronic signature. Printing or copy of file are considered as a copy of the document.

The reported uncertainty of measurement was based on standard uncertainty multiplied by a coverage factor (k) providing a level of confidence of approximately 95%. This certificate may not be reproduced other than in full except with the prior written approval of the Electrical and Electronics Institute, Foundation for Industrial Development.

Certificate No.: CP20240323EA

Calibration Report

Equipment: Sound Level Meter
Manufacturer: Larson Davis (Meter), PCB (Microphone), PCB (Preamplifier)
Model/Type: LxT1 (Meter), 377B02 (Microphone), PRMLxT1 (Preamplifier)
Serial No.: 0007305 (Meter), 345234 (Microphone), 077640 (Preamplifier)
ID No.: UAE.EFM.038/2566
Ambient Temperature: (23 ± 2) °C
Relative Humidity: (50 ± 15) %
Pressure: (101.3 ± 1.5) kPa
Method of Calibration :-
IEC 61672-3:2013.

Condition of this result of calibration

1. Reference standards instrument :-

	Instrument	Model	Serial No.	Cert. No.	Due Date
1)	Standard microphone	4180	2787490	AA-1012-23	12 November 2024
2)	Arbitrary Function Generator	AFG2021	C010063	CK20240048EA	23 June 2025
3)	Programmable Attenuator	PA5	2755	EF-0040-23	1 October 2024
4)	6.5 Digit precision multimeter	8846A	9610014	CB20230200EA	15 November 2024
5)	Pressure humidity and Temperature Transmitter	PTU301	L3950483	CL1-P240023 CD20240142EA	24 March 2025 12 June 2025
6)	Pressure humidity and Temperature Transmitter	PTU301	L3950484	CL1-P240030 CD20240143EA	11 April 2025 12 June 2025
7)	Performance Audio Analyzer	U8903B	MY56510003	CB20240035EB CK20230072EA	13 February 2025 13 September 2024

2. This result of calibration was found accurate as shown on date and place of calibration only.

3. This certification is traceable to the international system of unit maintained at :-

Reference standards instrument for Acoustic function

- National Institute of Metrology (Thailand)

Reference standards instrument for Electrical function

- National Institute of Metrology (Thailand)

- Electrical and Electronics Institute; NSC Accredited Calibration No.0119

Result of Calibration:-

Function : 1. Indication at the calibration check frequency

Reference Acoustic Signal (dB)	Measured value (dB)	Deviation (dB)	Acceptance limits (dB)
-	-	-	-

Certificate No.: CP20240323EA

Calibration Report

Function : 2. Self-generated Noise

2.1 Microphone Installed

Measured value (dB)
30.1

2.2 Microphone replaced by the electrical input signal device

Frequency Weighting	Measured value (dB)
A-weighting	29.9
C-weighting	30.0
Z-weighting	35.5

Function : 3. Acoustical signal tests of frequency weightings (Without Windscreen)

Meter free-field acoustic response at a level of 84 dB.

Frequency (Hz)	Deviation from various Frequency Weighting Response Curve			
	C-Weighting (dB)	A-Weighting (dB)	Z-Weighting (dB)	Acceptance limits (dB)
125	0.2	0.1	0.1	±1.0
1000	-0.1	-0.1	-0.1	±0.7
8000	0.6	0.5	0.6	+1.5; -2.5

Function : 4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various Frequency Weighting Response Curve			
	C-Weighting (dB)	A-Weighting (dB)	Z-Weighting (dB)	Acceptance limits (dB)
63	0.0	-0.1	0.0	±1.0
125	0.0	-0.1	0.0	±1.0
250	0.0	-0.1	0.0	±1.0
500	0.0	-0.1	0.0	±1.0
1000	0.0	0.0	0.0	±0.7
2000	0.0	-0.1	0.0	±1.0
4000	0.0	-0.1	0.0	±1.0
8000	-0.1	-0.1	0.0	+1.5; -2.5
16000	0.0	0.0	0.0	+2.5; -16.0

Certificate No.: CP20240323EA

Calibration Report

Function : 5. Frequency and time weighting at 1 kHz

5.1 Frequency weighting at 1 kHz

Frequency Weighting	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
C-weighting	94.0	0.0	±0.2
A-weighting	94.0	0.0	±0.2
Z-weighting	94.0	0.0	±0.2

5.2 Time weighting at 1 kHz

Time Weighting	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
Fast	94.0	0.0	±0.1
Slow	94.0	0.0	±0.1
LAeq	94.0	0.0	±0.1

Function : 6. Long-Term Stability

Long-term stability over 30 minutes, with steady 1 kHz signal at reference level.

Time Period to Apply Signal (min)	Reference SPL (dB)	Record SPL at Conclusion of Time Period (dB)	Deviated value (dB)	Acceptance limits (dB)
30	94.0	94.0	0.0	±0.1

Function : 7. Level Linearity on the reference level range

7.1 Level Linearity on the reference level range, Upper

Anticipated Value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
94.0	94.0	0.0	±0.8
99.0	99.0	0.0	±0.8
104.0	104.0	0.0	±0.8
109.0	109.0	0.0	±0.8
114.0	114.0	0.0	±0.8
119.0	119.0	0.0	±0.8
124.0	124.0	0.0	±0.8
129.0	129.0	0.0	±0.8
134.0	134.0	0.0	±0.8
139.0	139.0	0.0	±0.8
140.0	140.0	0.0	±0.8
141.0	141.0	0.0	±0.8

Certificate No.: CP20240323EA

Calibration Report

7.2 Level Linearity on the reference level range, Lower

Anticipated Value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
94.0	94.0	0.0	±0.8
89.0	89.0	0.0	±0.8
84.0	84.0	0.0	±0.8
79.0	79.0	0.0	±0.8
74.0	74.0	0.0	±0.8
69.0	69.0	0.0	±0.8
64.0	64.0	0.0	±0.8
59.0	59.0	0.0	±0.8
54.0	54.0	0.0	±0.8
49.0	49.0	0.0	±0.8
44.0	44.1	0.1	±0.8
39.0	39.4	0.4	±0.8

Function : 8. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
Fast	200	136.0	0.0	±0.5
	2	118.9	-0.1	+1.0 ; -1.5
	0.25	109.7	-0.3	+1.0 ; -3.0
Slow	200	129.5	-0.1	±0.5
	2	109.9	-0.1	+1.0 ; -3.0
	0.25	100.9	-0.1	+1.0 ; -3.0
LAE	200	130.0	0.0	±0.5
	2	110.0	0.0	+1.0 ; -1.5
	0.25	100.9	-0.1	+1.0 ; -3.0

Function : 9. Peak C sound level

Number of cycles in test signal	Anticipated Value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
Complete cycle	135.4	134.8	-0.6	±2.0
Positive half cycle	134.4	134.0	-0.4	±1.0
Negative half cycle	134.4	134.0	-0.4	±1.0

Certificate No.: CP20240323EA

Calibration Report

Function : 10. Overload indication

Measured value (dB)		Deviated value (dB)	Acceptance limits (dB)
Positive one-half cycle	Negative one-half cycle		
143.7	143.7	0.0	±1.5

Function : 11. High-Level Stability

High-level stability over 5 minutes, with steady 1 kHz signal, 1 dB below upper boundary.

Time Period to Apply Signal (min)	Reference SPL (dB)	Record SPL at Conclusion of Time Period (dB)	Deviated value (dB)	Acceptance limits (dB)
5	139.0	139.0	0.0	±0.1

Uncertainty of measurement

Function	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1) Indication at the calibration check frequency	0.30	Not applicable
2) Self-generated Noise	0.10	Not applicable
3) Acoustical signal tests of frequency weightings - Free-field sound pressure response level	0.30	0.60 (10Hz to 4kHz) 0.70 (>4kHz to 10kHz)
4) Electrical signal tests of frequency weightings	0.20	0.20
5) Frequency and time weighting at 1 kHz	0.20	0.20
6) Long-Term Stability	0.10	0.10
7) Level Linearity on the reference level range	0.30	0.30
8) Tone burst response	0.20	0.30
9) Peak C sound level	0.20	0.35
10) Overload indication	0.20	0.25
11) High-Level Stability	0.10	0.10

- Remarks:
1. Indication at the calibration check frequency can not measured because customer does not provide a sound calibrator.
 2. The acceptance limit is for the deviated value.
 3. Acceptance limits was IEC61672-3:2013 Class 1.
 4. The coverage factor $k = 2.00$

-- End of Report --

เอกสารไม่ควบคุม

Certificate No.: CP20240290EA
Operation No.: CP2024070253

Certificate of Calibration

Equipment: Sound Level Meter

Manufacturer: Larson Davis (Meter), PCB (Microphone), PCB (Preamplifier)

Model/Type: LxT1 (Meter), 377B02 (Microphone), PRMLxT1 (Preamplifier)

Serial No.: 0007306 (Meter), 345235 (Microphone), 077641 (Preamplifier)

ID No.: UAE.EFM.039/2566

Customer: United Analyst and Engineering Consultant Co.,Ltd.

Address: 81 Soi Udomsuk 41, Sukhumvit Road, Bangchak
Phrakhanong, Bangkok 10260

Received Date: 25 July 2024

Calibrated Date: 5 - 6 August 2024

Issued Date: 7 August 2024

Calibrated by: Ms. Juntaporn Kunhakom

Approved by: _____

Group Manager

This report was prepared electronically using applicable electronic signature. Printing or copy of file are considered as a copy of the document.

The reported uncertainty of measurement was based on standard uncertainty multiplied by a coverage factor (k) providing a level of confidence of approximately 95%. This certificate may not be reproduced other than in full except with the prior written approval of the Electrical and Electronics Institute, Foundation for Industrial Development.

Certificate No.: CP20240290EA

Calibration Report

Equipment: Sound Level Meter
 Manufacturer: Larson Davis (Meter), PCB (Microphone), PCB (Preamplifier)
 Model/Type: LxT1 (Meter), 377B02 (Microphone), PRMLxT1 (Preamplifier)
 Serial No.: 0007306 (Meter), 345235 (Microphone), 077641 (Preamplifier)
 ID No.: UAE.EFM.039/2566
 Ambient Temperature: (23 ± 2) °C
 Relative Humidity: (50 ± 15) %
 Pressure: (101.3 ± 1.5) kPa
 Method of Calibration :-
 IEC 61672-3:2013.

Condition of this result of calibration

1. Reference standards instrument :-

	Instrument	Model	Serial No.	Cert. No.	Due Date
1)	Standard microphone	4180	2787490	AA-1012-23	12 November 2024
2)	Arbitrary Function Generator	AFG2021	C010063	CK20240048EA	23 June 2025
3)	Programmable Attenuator	PA5	2755	EF-0040-23	1 October 2024
4)	6.5 Digit precision multimeter	8846A	9610014	CB20230200EA	15 November 2024
5)	Pressure humidity and Temperature Transmitter	PTU301	L3950483	CL1-P240023 CD20240142EA	24 March 2025 12 June 2025
6)	Pressure humidity and Temperature Transmitter	PTU301	L3950484	CL1-P240030 CD20240143EA	11 April 2025 12 June 2025
7)	Performance Audio Analyzer	U8903B	MY56510003	CB20240035EB CK20230072EA	13 February 2025 13 September 2024

2. This result of calibration was found accurate as shown on date and place of calibration only.

3. This certification is traceable to the international system of unit maintained at :-

Reference standards instrument for Acoustic function

- National Institute of Metrology (Thailand)

Reference standards instrument for Electrical function

- National Institute of Metrology (Thailand)

- Electrical and Electronics Institute; NSC Accredited Calibration No.0119

Result of Calibration:-

Function : 1. Indication at the calibration check frequency

Reference Acoustic Signal (dB)	Measured value (dB)	Deviation (dB)	Acceptance limits (dB)
-	-	-	-

Certificate No.: CP20240290EA

Calibration Report

Function : 2. Self-generated Noise

2.1 Microphone Installed

Measured value (dB)
28.8

2.2 Microphone replaced by the electrical input signal device

Frequency Weighting	Measured value (dB)
A-weighting	28.7
C-weighting	28.4
Z-weighting	34.5

Function : 3. Acoustical signal tests of frequency weightings (Without Windscreen)

Meter free-field acoustic response at a level of 84 dB.

Frequency (Hz)	Deviation from various Frequency Weighting Response Curve			
	C-Weighting (dB)	A-Weighting (dB)	Z-Weighting (dB)	Acceptance limits (dB)
125	0.1	0.0	0.0	±1.0
1000	-0.1	-0.1	-0.1	±0.7
8000	-0.4	-0.5	-0.4	+1.5; -2.5

Function : 4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various Frequency Weighting Response Curve			
	C-Weighting (dB)	A-Weighting (dB)	Z-Weighting (dB)	Acceptance limits (dB)
63	0.0	0.0	0.0	±1.0
125	0.0	0.0	0.0	±1.0
250	0.0	0.0	0.0	±1.0
500	0.0	0.0	0.0	±1.0
1000	0.0	0.0	0.0	±0.7
2000	0.0	0.0	0.0	±1.0
4000	0.0	0.0	0.0	±1.0
8000	-0.1	-0.1	0.0	+1.5; -2.5
16000	0.0	0.0	0.0	+2.5; -16.0

Certificate No.: CP20240290EA

Calibration Report

Function : 5. Frequency and time weighting at 1 kHz

5.1 Frequency weighting at 1 kHz

Frequency Weighting	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
C-weighting	94.0	0.0	±0.2
A-weighting	94.0	0.0	±0.2
Z-weighting	94.0	0.0	±0.2

5.2 Time weighting at 1 kHz

Time Weighting	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
Fast	94.0	0.0	±0.1
Slow	94.0	0.0	±0.1
LAeq	94.0	0.0	±0.1

Function : 6. Long-Term Stability

Long-term stability over 30 minutes, with steady 1 kHz signal at reference level.

Time Period to Apply Signal (min)	Reference SPL (dB)	Record SPL at Conclusion of Time Period (dB)	Deviated value (dB)	Acceptance limits (dB)
30	94.0	94.0	0.0	±0.1

Function : 7. Level Linearity on the reference level range

7.1 Level Linearity on the reference level range, Upper

Anticipated Value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
94.0	94.0	0.0	±0.8
99.0	99.0	0.0	±0.8
104.0	104.0	0.0	±0.8
109.0	109.0	0.0	±0.8
114.0	114.0	0.0	±0.8
119.0	119.0	0.0	±0.8
124.0	124.0	0.0	±0.8
129.0	129.0	0.0	±0.8
134.0	134.0	0.0	±0.8
139.0	139.0	0.0	±0.8
140.0	140.0	0.0	±0.8

Certificate No.: CP20240290EA

Calibration Report

7.2 Level Linearity on the reference level range, Lower

Anticipated Value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
94.0	94.0	0.0	±0.8
89.0	89.0	0.0	±0.8
84.0	84.0	0.0	±0.8
79.0	79.0	0.0	±0.8
74.0	74.0	0.0	±0.8
69.0	69.0	0.0	±0.8
64.0	64.0	0.0	±0.8
59.0	59.0	0.0	±0.8
54.0	54.0	0.0	±0.8
49.0	49.0	0.0	±0.8
44.0	44.1	0.1	±0.8
39.0	39.4	0.4	±0.8

Function : 8. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
Fast	200	136.0	0.0	±0.5
	2	118.8	-0.2	+1.0 ; -1.5
	0.25	109.7	-0.3	+1.0 ; -3.0
Slow	200	129.5	-0.1	±0.5
	2	109.8	-0.2	+1.0 ; -3.0
	0.25	100.9	-0.1	+1.0 ; -3.0
LAE	200	130.0	0.0	±0.5
	2	110.0	0.0	+1.0 ; -1.5
	0.25	100.9	-0.1	+1.0 ; -3.0

Function : 9. Peak C sound level

Number of cycles in test signal	Anticipated Value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
Complete cycle	135.4	134.8	-0.6	±2.0
Positive half cycle	134.4	134.0	-0.4	±1.0
Negative half cycle	134.4	134.0	-0.4	±1.0

Certificate No.: CP20240290EA

Calibration Report

Function : 10. Overload indication

Measured value (dB)		Deviated value (dB)	Acceptance limits (dB)
Positive one-half cycle	Negative one-half cycle		
142.6	142.6	0.0	±1.5

Function : 11. High-Level Stability

High-level stability over 5 minutes, with steady 1 kHz signal, 1 dB below upper boundary.

Time Period to Apply Signal (min)	Reference SPL (dB)	Record SPL at Conclusion of Time Period (dB)	Deviated value (dB)	Acceptance limits (dB)
5	139.0	139.0	0.0	±0.1

Uncertainty of measurement

Function	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1) Indication at the calibration check frequency	0.30	Not applicable
2) Self-generated Noise	0.10	Not applicable
3) Acoustical signal tests of frequency weightings - Free-field sound pressure response level	0.30	0.60 (10Hz to 4kHz) 0.70 (>4kHz to 10kHz)
4) Electrical signal tests of frequency weightings	0.20	0.20
5) Frequency and time weighting at 1 kHz	0.20	0.20
6) Long-Term Stability	0.10	0.10
7) Level Linearity on the reference level range	0.30	0.30
8) Tone burst response	0.20	0.30
9) Peak C sound level	0.20	0.35
10) Overload indication	0.20	0.25
11) High-Level Stability	0.10	0.10

- Remarks:
1. Indication at the calibration check frequency can not measured because customer does not provide a sound calibrator.
 2. The acceptance limit is for the deviated value.
 3. Acceptance limits was IEC61672-3:2013 Class 1.
 4. The coverage factor $k = 2.00$

-- End of Report --

เอกสารไม่ควบคุม

Envi Equipment Service Co., Ltd.

110/254 Moo 3, Tumbon Bang Rak Phatthana, Amphur Bang Bua Thong, Nonthaburi 11110

Tel. 098 362 9152, 089 478 7885

E-mail: sales@envi-ees.com

Certificate No.: E24-080073

Page.: 1 of 6

CERTIFICATE OF CALIBRATION

Customer : United Analyst and Engineering Consultant Co., Ltd.

Address : 81 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260

Description of Equipment : Console meter

Manufacturer : Apex Instrument

Model Number : XC-572-V

Serial Number : 1904011

ID./Control No. : UAE.EFM 118/2562

Environment Conditions : Temperature (25 ± 2) °C
: Humidity (50 ± 15) % RH

Cal. Date : 21/08/2024

Issue Date : 21/08/2024

Calibration Method or Calibration Procedure Used

US EPA Method (United State Environmental Protection Agency)

This certificate is traceable to national standard, which realize the units of measurement according to the International System of Units (IS).

Result of Calibration

This certificate may not be reproduced other than in full except with prior Written approval of the Technical Manager, Envi Equipment Service Company Limited.

These reported uncertainties of measurement are expanded by a coverage factor of k=2, providing a 95% confidence level

Calibrated by : 

Approved by : 



Technical Manager

เอกสารไม่ควบคุม

**METHOD 5 CONSOLE CALIBRATION
USING REFERENCE WET GAS METER W-NK-2.5-B-Z No.547425
5-POINT METRIC UNIT**

Meter Console Information		Calibration Conditions				Factors/Conversions		
Console Model Number	XC-572-V	Date	Time	21/08/2024	10:00 AM	Std Temp	293	K
Console Serial Number	1904011	Calibration Reference No.		SER24-070026		Std Press	760	mm Hg
DGM Model Number	SK25EX	Barometric Pressure		758.16	mmHg	K ₁	0.386	
DGM Serial Number	00008685	Calibration Meter Gamma		1.001		Console Leak Check		PASS

Calibration Data									
Run Time	Metering Console					Calibration Meter			
Elapsed	DGM Orifice DH	Volume Initial	Volume Final	Outlet Temp Initial	Outlet Temp Final	Volume Initial	Volume Final	Outlet Temp Initial	Outlet Temp Final
(Q)	(P _m)	(V _{mi})	(V _{mf})	(t _{mi})	(t _{mf})	(V _{wi})	(V _{wf})	(t _{wi})	(t _{wf})
min	mm H ₂ O	m ³	m ³	°C	°C	m ³	m ³	°C	°C
11.97	13.0	1.2810	1.4210	30	30	247.58494	247.72266	28	28
12.02	13.0	1.4210	1.5610	30	30	247.72266	247.86142	27	27
8.43	26.0	1.5680	1.7080	29	29	247.86722	248.00508	27	27
8.40	26.0	1.7080	1.8480	29	29	248.00508	248.14262	26	26
13.78	40.0	1.8550	2.1350	29	29	248.15146	248.42930	26	26
13.82	40.0	2.1350	2.4150	29	29	248.42930	248.70800	26	26
10.28	70.0	2.4270	2.7070	30	30	248.71530	248.99226	25	25
10.33	70.0	2.7070	2.9870	30	30	248.99226	249.27106	25	25
8.95	90.0	3.0020	3.2820	31	31	249.27896	249.55508	25	25
8.92	90.0	3.2820	3.5620	31	31	249.55508	249.83062	25	25



เอกสารไม่ควบคุม

**METHOD 5 CONSOLE CALIBRATION
USING REFERENCE WET GAS METER W-NK-2.5-B-Z No.547425
5-POINT METRIC UNIT**

Meter Console Information		Calibration Conditions				Factors/Conversions		
Console Model Number	XC-572-V	Date	Time	21/08/2024	10:00 AM	Std Temp	293	K
Console Serial Number	1904011	Calibration Reference No.		SER24-070026		Std Press	760	mm Hg
DGM Model Number	SK25EX	Barometric Pressure		758.16	mm Hg	K ₁	0.386	
DGM Serial Number	00008685	Calibration Meter Gamma		1.001		Console Leak Check		PASS

Calibration Data								
Results								
Standardized Data				Dry Gas Meter				
Dry Gas Meter		Calibration Meter		Calibration Factor		Flowrate		
(V _{m(std)})	(Q _{m(std)})	(V _{w(std)})	(Q _{w(std)})	Value	Variation	Std & Corr	.0212 m ³ _{std} /min	Variation
m ³	m ³ /min	m ³	m ³ /min	(Y)	(ΔY)	(Q _{m(std)(corr)})	(ΔH _@)	(ΔH _@)
						m ³ /min	mm H ₂ O	
0.136	0.011	0.134	0.011	0.981	-0.001	0.011	45.783	0.623
0.137	0.011	0.135	0.011	0.989	0.006	0.011	45.326	0.166
0.137	0.016	0.134	0.016	0.981	-0.002	0.016	45.347	0.187
0.137	0.016	0.134	0.016	0.979	-0.004	0.016	45.048	-0.112
0.275	0.020	0.271	0.020	0.987	0.005	0.020	45.852	0.692
0.275	0.020	0.272	0.020	0.991	0.008	0.020	45.790	0.630
0.276	0.027	0.271	0.026	0.981	-0.001	0.026	45.058	-0.102
0.276	0.027	0.273	0.026	0.988	0.005	0.026	44.899	-0.261
0.277	0.031	0.271	0.030	0.977	-0.006	0.030	44.320	-0.840
0.277	0.031	0.270	0.030	0.975	-0.008	0.030	44.176	-0.984
				0.983	Y Average		45.160	ΔH@ Average

Note: For Calibration Factor Y, the ratio of the reading of the calibration meter to the dry gas meter, acceptable tolerance of individual values from the average is ±0.02.

For ΔH_@, orifice pressure differential that equates to 0.75 cfm (0.0212 m³/min) at standard temperature and pressure, acceptable tolerance of individual values from the average is ±0.2 inches (5.1mm) H₂O.



เอกสารไม่ควบคุม

Meter Console Information	
Console Model Number	XC-572-V
Console Serial Number	1904011
DGM Model Number	SK25EX
DGM Serial Number	00008685


Calibration Conditions			
Date	Time	21/08/2024	10:00 AM
Calibration Reference No.	SER24-070026		
Barometric Pressure	758.16	mmHg	
Calibration Meter Gamma	1.001		

Factors/Conversions		
Std Temp	293	K
Std Press	760	mm Hg
K ₁	0.386	
Console Leak Check	PASS	

Calibration Date: 21-8-2024

Calibration Reference No: SER24-070026

Meter Gamma vs Flowrate

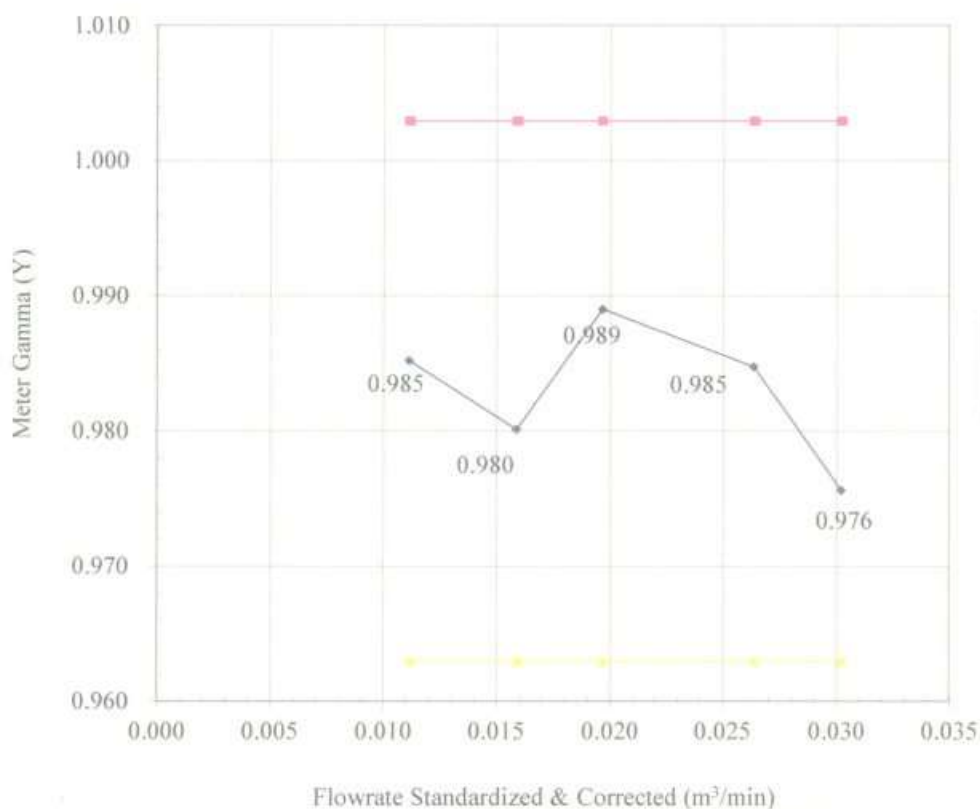

Console Serial: 1904011

Console Model: XC-572-V



เอกสารไม่ควบคุม

Meter Console Information	
Console Model Number	XC-572-V
Console Serial Number	1904011
DGM Model Number	SK25EX
DGM Serial Number	00008685


Calibration Conditions			
Date	Time	21/08/2024	10:00 AM
Calibration Reference No.		SER24-070026	
Barometric Pressure		758.16	mmHg
Calibration Meter Gamma		1.001	

Factors/Conversions		
Std Temp	293	K
Std Press	760	mm Hg
K _t	0.386	
Console Leak Check		PASS

Calibration Date: 21-8-2024

Calibration Reference No: SER24-070026

Meter Pressure vs Flowrate

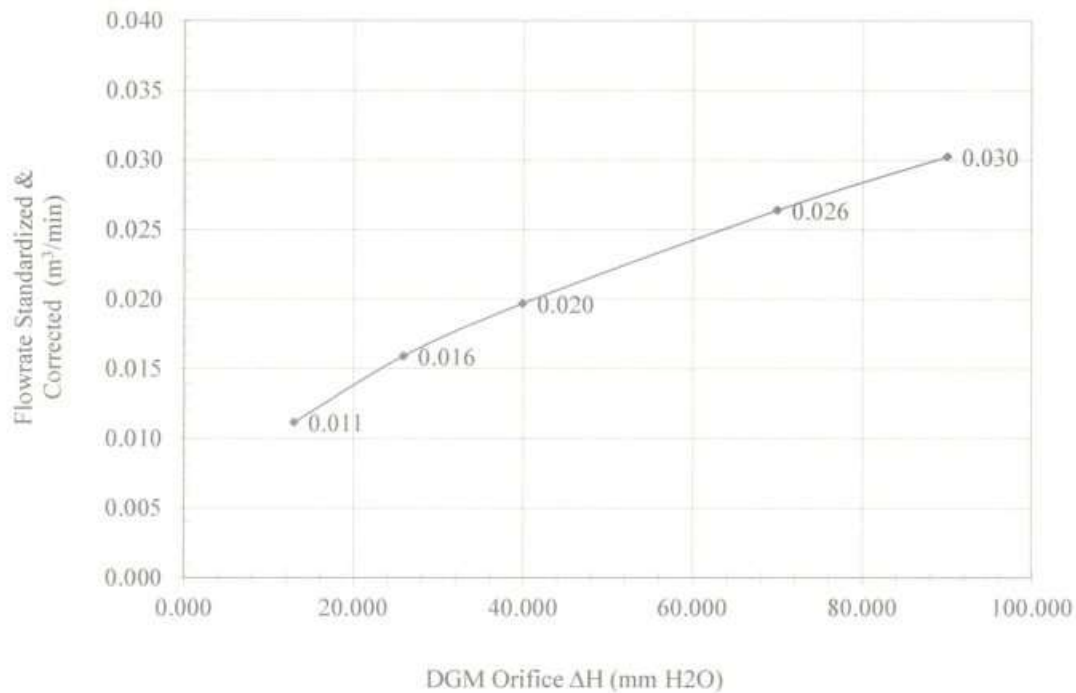

Console Serial: 1904011

Console Model: XC-572-V



เอกสารไม่ควบคุม

THERMOCOUPLES SYSTEM CALIBRATION

Sampling System Equipment Information	
Console Model Number	XC-572-V
Console Serial Number	1904011
DGM Model Number	SK25EX
DGM Serial Number	00008685
Meter Box Model Number	JENCO 765 KF
Meter Box Serial Number	JC 17215

Calibration Conditions			
Date	Time	21/08/2024	00:00 PM
Calibration Reference No.	SER24-070026		
Reference Thermometer	DIGICON		
Serial Number	183169105		

Results											
Console Thermocouple Simulator											
Channel and test point	Meter Box Channel Temperature Reading (°C)										
	-18.0	25.0	38.0	93.0	149.0	260.0	371.0	482.0	593.0	816.0	1038.0
Stack	-19.0	24.0	37.0	93.0	148.0	257.0	368.0	477.0	586.0	805.0	1025.0
Aux	-19.0	24.0	37.0	93.0	148.0						
Probe	-19.0	24.0	37.0	93.0	148.0						
Filter	-19.0	24.0	37.0	93.0	148.0						
Oven	-19.0	24.0	37.0	93.0	148.0						
Exit	-19.0	24.0	37.0								

Tolerance Range

Stack ± 1.50% Absolute
 Probe ± 3.0 °C
 Filter ± 3.0 °C

Meter ± 3.0 °C
 Exit ± 2.0 °C



เอกสารไม่ควบคุม

Certificate No: G 670083

Date of issue : 08-Feb-24

Instrument description : Flue Gas Analyzer
Instrument model : Testo 350 New
Control unit serial no. : 03099393/701
Instrument serial no. : 60899698/701
ID no. or control no. : UAE.EFM.008/2560
Manufacturer : Testo SE & Co. KGaA
Probe description : -
Probe model : -
Probe serial no. : -
Customer name : UNITED ANALYST CONSULTANT CO.,LTD.
Customer address : 81 SOI UDOMSUK41,SUKHUMVIT ROAD,BANGCHAK PRAKANONG BANGKOK 10260

Total pages of certificate : 2 Pages
Receiving no. : L-240430
Receiving date. : 05-Feb-24
Parameter of calibration : Gas Calibration(Oxygen 2.50,10.04,21.02 %vol, Carbon Monoxide 80.14,302,1003 ppm, Nitrogen Dioxide 30.34,81.32, 201.9 ppm, Nitric Oxide 30.01, 151.5, 322.5 ppm, Sulphur Dioxide 50.36, 100.8, 600.8 ppm)
Condition of UUC. : Used
Ambient condition : All of the Measurment ware caried out the stabilized labotary
 Temperature : 23 ±5 °C
 Humidity : 55 ± 15 %RH
Calibration place : 17/121 Soi Ngamwongwan 47 Yaek 48, Toongsonghong, Laksi, Bangkok 10210
Calibration procedure no. : This instrument was calibrated by comparison with Standard gas mixture according to calibration Work Instruction no. WI-CL-28-C

The calibration certificate expanded uncertainty of measurement is stated as the standard uncertainty of measurent Multiplied by coverage factor $k=2$, which for a normal distribution corresponds to a coverage probability of approximately 95%.

This certificate is applied only to item under test Environmental condition.


This Calibration Certificate may not be reporduced other than in full except with the permission of the issuing laboratory. Calibration certificates without signature and seal not valid and The results relate only to the items tested/calibrated.

This calibration certificate documents are tracebility to national standards, which realize measurement according to the International System of Units (SI).

Date of calibration : 08-Feb-24



Calibration Technician



Technical Manager

Certificate No.: G 670083

Standard References (Table 1)

Standard	Certificate No.	Vendor	Due date
Oxygen (O ₂) 2.50 % Vol	2412/23	Linde	27-Aug-27
Oxygen (O ₂) 10.04 % Vol	CG-0153-21	Nimt	18-Nov-26
Oxygen (O ₂) 21.02 % Vol	CG-0041-22	Nimt	10-Feb-27
Carbon monoxide (CO) 80.14 ppm	CG-0040-22	Nimt	14-Feb-27
Carbon monoxide (CO) 302 ppm	1915/23	Linde	16-Jun-25
Carbon monoxide (CO) 1003 ppm	2584/23	Linde	10-Sep-25
Nitrogen Dioxide (NO ₂) 30.34 ppm	2703/22	Linde	22-Aug-24
Nitrogen Dioxide (NO ₂) 81.32 ppm	3546/23	Linde	14-Jan-26
Nitrogen Dioxide (NO ₂) 201.9 ppm	1975/23	Linde	17-Jul-25
Nitric Oxide (NO) 30.01 ppm	CG-0014-23	Nimt	19-Feb-25
Nitric Oxide (NO) 151.5 ppm	0161/23	Linde	22-Jan-25
Nitric Oxide (NO) 322.5 ppm	1974/23	Linde	17-Jul-25
Sulphur Dioxide (SO ₂) 50.36 ppm	2004/23	Linde	17-Jul-25
Sulphur Dioxide (SO ₂) 100.8 ppm	3507/22	Linde	09-Nov-24
Sulphur Dioxide (SO ₂) 600.8 ppm	2003/23	Linde	17-Jul-25

Measured room conditions

Temperature : 23.5 °C Humidity : 64.1 %RH Pressure : 1011.7 mbar

Calibration conditions

Gas Temperature : 23 °C Flow rate : 1,200 ml/min Gas pressure : 1016.4 mbar

Calibration Results (Without adjustment) (Table 2)

Parameter of Standard	Standard Values	Mean of UUC	Error	Uncertainty (±)
O ₂ (%Vol)	2.50	2.57	0.07	0.15
O ₂ (%Vol)	10.04	10.09	0.05	0.20
O ₂ (%Vol)	21.02	21.08	0.06	0.30
CO (ppm)	80.14	81	0.86	3.0
CO (ppm)	302	302	0	6.0
CO (ppm)	1003	1002	-1	12
NO ₂ (ppm)	30.34	30.2	0.14	8.0
NO ₂ (ppm)	81.32	82.4	1.08	8.0
NO ₂ (ppm)	201.9	202.8	0.9	12
NO (ppm)	30.01	29	-1.01	8.0
NO (ppm)	151.5	150	-1.5	8.0
NO (ppm)	322.5	320	-2.5	12
SO ₂ (ppm)	50.36	49	-1.36	6.0
SO ₂ (ppm)	100.8	100	-0.8	6.0
SO ₂ (ppm)	600.8	599	-1.8	13

Remark : 1 cmol/mol = 1 %vol. 1 μmol/mol = 1 ppm.

End of Report

Cert. No. : ACL24051

Pages : 1 of 8

Calibration Certificate

Equipment : SOUND LEVEL METER
Manufacturer : RION
Model : NL-42 / Microphone UC-52 / Preamplifier NH-24
Serial No.: 00408982 / 186172 / 00727
ID No.: UAE.EFM.009/2564

Condition As Found : GOOD

Customer : UNITED ANALYST AND ENGINEERING CONSULTANT (UAE)
81 SOI UDOMSUK 41, SUKHUMVIT ROAD,
BANGCHAK SUB-DISTRICT,
PHRAKHANONG DISTRICT, BANGKOK 10260
THAILAND.


Location : -
Ambient Temperature : (23.0 \pm 3) °C
Pressure : (101.3 \pm 3) kPa
Relative Humidity : (50.0 \pm 20) %

Received Date : 21 DECEMBER 2023
Calibration Date : 18-19 JANUARY 2024
Date of Issue : 22 JANUARY 2024

Calibrated by :



Approved by :



This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

เอกสารไม่ควบคุม

SITHIPORN ASSOCIATES CO., LTD.

CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand
Tel. +66 2433 8331 Email : calibration@sithiporn.com



Cert. No. : ACL24051
Job No. : VC67AC0034
Pages : 2 of 8

Calibration Procedure : CP-AC-01

Calibration Method :

This equipment was calibrated by follow on IEC-61672-3 (2013) Standard for sound level meter (SLM).
The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.
For tests results of each items were made by observation of each Instruments display and also with SLM's display.

Condition of this result of calibration :

1. Reference Standard Instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
Waveform Generator	33210A	MY48017076	EF-0009-23	07-FEB-24
Waveform Generator	33511B	MY52302742	EF-0010-23	07-FEB-24
Digital Multimeter	33461A	MY53220104	EEL.BP 30/0266	13-FEB-24
Digital Multimeter	33461A	MY53220076	EEL.BP 29/0266	13-FEB-24
Digital Multimeter	34461A	MY60024273	EEL.BP 31/0266	14-FEB-24
Programmable Attenuator	MAT-1070	62100114	EF-0011-23	08-FEB-24
Condenser Microphone	4180	2977900	AA-1001-23	14-FEB-24
Measuring Amplifier	NA-42KAI	34560495	AA-3002-23	14-FEB-24

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.
3. This certificate is traceable to the international system of unit maintained at :
 - 3.1 National Institute of Metrology (Thailand).
 - 3.2 Thailand Institute of Scientific and Technological Research (TISTR).

เอกสารนี้เป็นเอกสารของบริษัท

SITHIPORN ASSOCIATES CO., LTD.

CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbunru, Bangplud, Bangkok, 10700 Thailand
Tel. +66 2433 8331 Email : calibration@sithiporn.com

SITHIPORN
associates



Cert. No. : ACL24051
Job No. : VC67AC0034
Pages : 3 of 8

Summary of Measurement Result :

Parameter	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	0.2	N/A
2. Self-generated noise	0.2	N/A
3. Acoustical signal tests of frequency weightings		
125 Hz	0.3	0.6
1000 Hz	0.3	0.6
8000 Hz	0.3	0.7
4. Electrical signal tests of frequency weightings		
For 10 Hz to 4 kHz	0.3	0.6
For > 4 kHz to 10 kHz	0.3	0.7
For > 10 kHz to 20 kHz	-	1.0
5. Frequency and time weightings at 1 kHz	0.2	0.2
6. Long - term stability	0.1	0.1
7. Level linearity on the reference level range	0.2	0.3
8. Level linearity including the level range control	0.2	0.3
9. Tone burst response	0.2	0.3
10. Peak C sound level	0.2	0.35
11. Overload indication	0.2	0.25
12. High level stability	0.1	0.1

10

Cert. No. : ACL24051

Job No. : VC67AC0034

Pages : 4 of 8

Result of calibration :

1. Absolute sensitivity

Reference Acoustic Signal (dB)	Measured Value (dB)	Deviation (dB)	Acceptance Limit (dB)
93.9 (93.98)	93.9	0.0	±0.3

2. Self-generated noise

2.1 Normal test

Measured Value (dB)
14.8

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Measured value (dB)
A - weight	12.6
C - weight	19.2
Flat	24.7

3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
125	0.0	0.1	0.1	± 1.5
1000	0.0	0.0	0.0	± 1.0
8000	2.3	2.4	2.4	±5.0

Cert. No. : ACL24051
Job No. : VC67AC0034
Pages : 5 of 8

4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	-0.1	0.0	0.0	±2.0
125	0.0	0.0	0.0	±1.5
250	0.0	0.0	0.0	±1.5
500	0.0	0.1	0.0	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.1	0.0	±2.0
4000	0.0	0.0	0.0	±3.0
8000	0.0	0.1	0.1	±5.0

5. Frequency and time weightings at 1 kHz

5.1 Frequency weightings at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.2
C - weight	94.0	94.0	0.0	± 0.2
Flat	94.0	94.0	0.0	± 0.2

5.2 Time weighting at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	94.0	94.0	0.0	± 0.1
Slow	94.0	94.0	0.0	± 0.1
Leq	94.0	94.0	0.0	± 0.1

6. Long - term stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.2

เอกสารไม่ควบคุม

SITHIPORN ASSOCIATES CO., LTD.

CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand
Tel. +66 2433 8331 Email : calibration@sithiporn.com

SITHIPORN
associates



Cert. No. : ACL24051

Job No. : VC67AC0034

Pages : 6 of 8

7. Level linearity on the reference level range

Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
137.0	137.0	0.0	± 1.1
136.0	136.0	0.0	± 1.1
135.0	135.0	0.0	± 1.1
134.0	134.0	0.0	± 1.1
133.0	133.0	0.0	± 1.1
132.0	132.0	0.0	± 1.1
131.0	131.0	0.0	± 1.1
129.0	129.0	0.0	± 1.1
124.0	124.0	0.0	± 1.1
119.0	119.0	0.0	± 1.1
114.0	114.0	0.0	± 1.1
109.0	109.0	0.0	± 1.1
104.0	104.0	0.0	± 1.1
99.0	99.0	0.0	± 1.1
94.0	94.0	0.0	± 1.1
89.0	89.0	0.0	± 1.1
84.0	84.0	0.0	± 1.1
79.0	79.0	0.0	± 1.1
74.0	74.0	0.0	± 1.1
69.0	69.0	0.0	± 1.1
64.0	64.0	0.0	± 1.1
59.0	59.0	0.0	± 1.1
54.0	54.0	0.0	± 1.1
49.0	49.0	0.0	± 1.1
44.0	44.0	0.0	± 1.1
39.0	39.0	0.0	± 1.1
34.0	34.0	0.0	± 1.1
30.0	29.9	-0.1	± 1.1
29.0	28.9	-0.1	± 1.1
28.0	27.9	-0.1	± 1.1
27.0	26.9	-0.1	± 1.1
26.0	25.9	-0.1	± 1.1
25.0	24.9	-0.1	± 1.1

เอกสารไม่ควบคุม
7. Relu.

Cert. No. : ACL24051
Job No. : VC67AC0034
Pages : 7 of 8

8. Level linearity including the level range control

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Auto	94.0	94.0	0.0	±1.1

9. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Cycle	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.1	0.1	±1.0
Slow	2	8	108.0	108.0	0.0	1.5 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
SEL	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.1	0.1	±1.0

10. Peak C sound level

Number of cycle in test signal	Anticipated Value (dB)	Measured Value, Lcpeak (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	±3.0
One	136.4	136.3	-0.1	±3.0

Number of cycle in test signal	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	±2.0
Positive half cycle	135.4	135.2	-0.2	±2.0
Negative half cycle	135.4	135.2	-0.2	±2.0

SITHIPORN ASSOCIATES CO., LTD.

CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand
Tel. +66 2433 8331 Email : calibration@sithiporn.com

SITHIPORN
associates



Cert. No. : ACL24051
Job No. : VC67AC0034
Pages : 8 of 8

11. Overload indication

Measured value (dB)		Deviated Value (dB)	Acceptance Limits (dB)
Positive one-half cycle	Negative one-half cycle		
89.6	89.5	-0.1	±1.5

12. High level stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor $k = 2$
or any value following calculation, providing a level of confidence of approximately 95 %

End of Calibration Certificate

เอกสารไม่ควบคุม

Cert. No. : ACL24060

Pages : 1 of 8

Calibration Certificate

Equipment : SOUND LEVEL METER
Manufacturer : RION
Model : NL-42 / Microphone UC-52 / Preamplifier NH-24
Serial No.: 00709655 / 188530 / 01206
ID No.: UAE.EFM.020/2564

Condition As Found : GOOD

Customer : UNITED ANALYST AND ENGINEERING CONSULTANT (UAE)
81 SOI UDOMSUK 41, SUKHUMVIT ROAD,
BANGCHAK SUB-DISTRICT,
PHRAKHANONG DISTRICT, BANGKOK 10260
THAILAND.

Location : -

Ambient Temperature : (23.0 \pm 3) °C
Pressure : (101.3 \pm 3) kPa
Relative Humidity : (50.0 \pm 20) %

Received Date : 21 DECEMBER 2023
Calibration Date : 18-19 JANUARY 2024
Date of Issue : 22 JANUARY 2024

Calibrated by :

Nathakorn Pisutpaisan

Approved by :



This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

เอกสารไม่ควบคุม

SITHIPORN ASSOCIATES CO., LTD. CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand
Tel. +66 2433 8331 Email : calibration@sithiporn.com

SITHIPORN
associates



Cert. No. : ACL24060
Job No. : VC67AC0034
Pages : 2 of 8

Calibration Procedure : CP-AC-01

Calibration Method :

This equipment was calibrated by follow on IEC-61672-3 (2013) Standard for sound level meter (SLM).

The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.

For tests results of each items were made by observation of each Instruments display and also with SLM's display.

Condition of this result of calibration :

1. Reference Standard Instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
Waveform Generator	33210A	MY48017076	EF-0009-23	07-FEB-24
Waveform Generator	33511B	MY52302742	EF-0010-23	07-FEB-24
Digital Multimeter	33461A	MY53220104	EEL.BP 30/0266	13-FEB-24
Digital Multimeter	33461A	MY53220076	EEL.BP 29/0266	13-FEB-24
Digital Multimeter	34461A	MY60024273	EEL.BP 31/0266	14-FEB-24
Programmable Attenuator	MAT-1070	62100114	EF-0011-23	08-FEB-24
Condenser Microphone	4180	2977900	AA-1001-23	14-FEB-24
Measuring Amplifier	NA-42KAI	34560495	AA-3002-23	14-FEB-24

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is traceable to the international system of unit maintained at :

3.1 National Institute of Metrology (Thailand).

3.2 Thailand Institute of Scientific and Technological Research (TISTR).

เอกสารไม่ควบคุม

SITHIPORN ASSOCIATES CO., LTD. CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbunru, Bangplud, Bangkok, 10700 Thailand
Tel. +66 2433 8331 Email : calibration@sithiporn.com

SITHIPORN
associates



Cert. No. : ACL24060
Job No. : VC67AC0034
Pages : 3 of 8

Summary of Measurement Result :

Parameter	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	0.2	N/A
2. Self-generated noise	0.2	N/A
3. Acoustical signal tests of frequency weightings		
125 Hz	0.3	0.6
1000 Hz	0.3	0.6
8000 Hz	0.3	0.7
4. Electrical signal tests of frequency weightings		
For 10 Hz to 4 kHz	0.3	0.6
For > 4 kHz to 10 kHz	0.3	0.7
For > 10 kHz to 20 kHz	-	1.0
5. Frequency and time weightings at 1 kHz	0.2	0.2
6. Long - term stability	0.1	0.1
7. Level linearity on the reference level range	0.2	0.3
8. Level linearity including the level range control	0.2	0.3
9. Tone burst response	0.2	0.3
10. Peak C sound level	0.2	0.35
11. Overload indication	0.2	0.25
12. High level stability	0.1	0.1

เอกสารนี้เป็นความลับ

Cert. No. : ACL24060

Job No. : VC67AC0034

Pages : 4 of 8

Result of calibration :

1. Absolute sensitivity

Reference Acoustic Signal (dB)	Measured Value (dB)	Deviation (dB)	Acceptance Limit (dB)
93.9 (93.98)	93.9	0.0	±0.3

2. Self-generated noise

2.1 Normal test

Measured Value (dB)
15.1

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Measured value (dB)
A - weight	11.6
C - weight	17.5
Flat	23.3

3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
125	0.2	0.2	0.2	± 1.5
1000	0.1	0.1	0.1	± 1.0
8000	2.1	2.2	2.2	±5.0

Cert. No. : ACL24060
Job No. : VC67AC0034
Pages : 5 of 8

4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	-0.1	-0.1	0.0	±2.0
125	0.0	0.0	0.0	±1.5
250	0.0	0.0	0.0	±1.5
500	0.0	0.0	0.0	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.0	0.0	±2.0
4000	0.0	0.0	0.0	±3.0
8000	0.0	0.1	0.1	±5.0

5. Frequency and time weightings at 1 kHz

5.1 Frequency weightings at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.2
C - weight	94.0	94.0	0.0	± 0.2
Flat	94.0	94.0	0.0	± 0.2

5.2 Time weighting at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	94.0	94.0	0.0	± 0.1
Slow	94.0	94.0	0.0	± 0.1
Leq	94.0	94.0	0.0	± 0.1

6. Long - term stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.2

เอกสารไม่ควบคุม

SITHIPORN ASSOCIATES CO., LTD. CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbunru, Bangplud, Bangkok, 10700 Thailand
Tel. +66 2433 8331 Email : calibration@sithiporn.com

SITHIPORN
associates



Cert. No. : ACL24060

Job No. : VC67AC0034

Pages : 6 of 8

7. Level linearity on the reference level range

Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
137.0	137.0	0.0	± 1.1
136.0	136.0	0.0	± 1.1
135.0	135.0	0.0	± 1.1
134.0	134.0	0.0	± 1.1
133.0	133.0	0.0	± 1.1
132.0	132.0	0.0	± 1.1
131.0	131.0	0.0	± 1.1
129.0	129.0	0.0	± 1.1
124.0	124.0	0.0	± 1.1
119.0	119.0	0.0	± 1.1
114.0	114.0	0.0	± 1.1
109.0	109.0	0.0	± 1.1
104.0	104.0	0.0	± 1.1
99.0	99.0	0.0	± 1.1
94.0	94.0	0.0	± 1.1
89.0	89.0	0.0	± 1.1
84.0	84.0	0.0	± 1.1
79.0	79.0	0.0	± 1.1
74.0	74.0	0.0	± 1.1
69.0	69.0	0.0	± 1.1
64.0	64.0	0.0	± 1.1
59.0	59.0	0.0	± 1.1
54.0	53.9	-0.1	± 1.1
49.0	49.0	0.0	± 1.1
44.0	44.0	0.0	± 1.1
39.0	38.9	-0.1	± 1.1
34.0	33.9	-0.1	± 1.1
30.0	29.9	-0.1	± 1.1
29.0	28.9	-0.1	± 1.1
28.0	27.9	-0.1	± 1.1
27.0	26.9	-0.1	± 1.1
26.0	25.9	-0.1	± 1.1
25.0	24.9	-0.1	± 1.1

เอกสารไม่ควบคุม

Cert. No. : ACL24060
Job No. : VC67AC0034
Pages : 7 of 8

8. Level linearity including the level range control

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Auto	94.0	94.0	0.0	±1.1

9. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Cycle	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.0	0.0	±1.0
Slow	2	8	108.0	108.0	0.0	1.5 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
SEL	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.1	0.1	±1.0

10. Peak C sound level

Number of cycle in test signal	Anticipated Value (dB)	Measured Value, Lcpeak (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	±3.0
One	136.4	136.2	-0.2	±3.0

Number of cycle in test signal	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	±2.0
Positive half cycle	135.4	135.2	-0.2	±2.0
Negative half cycle	135.4	135.2	-0.2	±2.0

เอกสารไม่ควบคุม

SITHIPORN ASSOCIATES CO., LTD. CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbunru, Bangplud, Bangkok, 10700 Thailand
Tel. +66 2433 8331 Email : calibration@sithiporn.com

SITHIPORN
associates



Cert. No. : ACL24060
Job No. : VC67AC0034
Pages : 8 of 8

11. Overload indication

Measured value (dB)		Deviated Value (dB)	Acceptance Limits (dB)
Positive one-half cycle	Negative one-half cycle		
89.6	89.6	0.0	±1.5

12. High level stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor $k = 2$
or any value following calculation, providing a level of confidence of approximately 95 %

————— End of Calibration Certificate —————

เอกสารไม่ควบคุม

Cert. No. : ACL24160

Pages : 1 of 8

Calibration Certificate

Equipment : SOUND LEVEL METER
Manufacturer : RION
Model : NL-42 / Microphone UC-52 / Preamplifier NH-24
Serial No.: 00409023 / 185669 / 90468
ID No.: UAE.EFM.011/2564

Condition As Found : GOOD

Customer : UNITED ANALYST AND ENGINEERING CONSULTANT (UAE)
81 SOI UDOMSUK 41, SUKHUMVIT ROAD,
BANGCHAK SUB-DISTRICT,
PHRAKHANONG DISTRICT, BANGKOK 10260
THAILAND.


Location : -
Ambient Temperature : (23.0 \pm 3) °C
Pressure : (101.3 \pm 3) kPa
Relative Humidity : (50.0 \pm 20) %

Received Date : 10 MAY 2024
Calibration Date : 04 - 05 JUNE 2024
Date of Issue : 06 JUNE 2024

Calibrated by :



Approved by :



This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

เอกสารไม่ควบคุม

SITHIPORN ASSOCIATES CO., LTD.

CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand
Tel. +66 2433 8331 Email : calibration@sithiporn.com

SITHIPORN
associates



Cert. No. : ACL24160

Job No. : VC67AC0071

Pages : 2 of 8

Calibration Procedure : CP-AC-01

Calibration Method :

This equipment was calibrated by follow on IEC-61672-3 (2013) Standard for sound level meter (SLM).

The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.

For tests results of each items were made by observation of each Instruments display and also with SLM's display.

Condition of this result of calibration :

1. Reference Standard Instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
Waveform Generator	33210A	MY48017076	EF-0009-24	05-FEB-25
Waveform Generator	33511B	MY52302742	EF-0007-24	05-FEB-25
Digital Multimeter	33461A	MY53220104	EEL.BP 21/0267	13-FEB-25
Digital Multimeter	33461A	MY53220076	EEL.BP 20/0267	15-FEB-25
Digital Multimeter	34461A	MY60024273	EEL.BP 22/0267	15-FEB-25
Programmable Attenuator	MAT-1070	62100114	EF-0008-24	05-FEB-25
Condenser Microphone	4180	2977900	AA-1001-24	12-FEB-25
Measuring Amplifier	NA-42KAI	34560495	AA-3001-24	05-FEB-25

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is traceable to the international system of unit maintained at :

3.1 National Institute of Metrology (Thailand).

3.2 Thailand Institute of Scientific and Technological Research (TISTR).

เอกสารไม่ควบคุม

SITHIPORN ASSOCIATES CO., LTD.

CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand
Tel. +66 2433 8331 Email : calibration@sithiporn.com

SITHIPORN
associates



Cert. No. : ACL24160
Job No. : VC67AC0071
Pages : 3 of 8

Summary of Measurement Result :

Parameter	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	0.2	N/A
2. Self-generated noise	0.2	N/A
3. Acoustical signal tests of frequency weightings		
125 Hz	0.3	0.6
1000 Hz	0.3	0.6
8000 Hz	0.3	0.7
4. Electrical signal tests of frequency weightings		
For 10 Hz to 4 kHz	0.3	0.6
For > 4 kHz to 10 kHz	0.3	0.7
For > 10 kHz to 20 kHz	-	1.0
5. Frequency and time weightings at 1 kHz	0.2	0.2
6. Long - term stability	0.1	0.1
7. Level linearity on the reference level range	0.2	0.3
8. Level linearity including the level range control	0.2	0.3
9. Tone burst response	0.2	0.3
10. Peak C sound level	0.2	0.35
11. Overload indication	0.2	0.25
12. High level stability	0.1	0.1

เอกสารนี้เป็นความลับ

SITHIPORN ASSOCIATES CO., LTD.

CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand
Tel. +66 2433 8331 Email : calibration@sithiporn.com

SITHIPORN
associates



Cert. No. : ACL24160

Job No. : VC67AC0071

Pages : 4 of 8

Result of calibration :

1. Absolute sensitivity

Reference Acoustic Signal (dB)	Measured Value (dB)	Deviation (dB)	Acceptance Limit (dB)
93.9 (93.94)	93.9	0.0	±0.3

2. Self-generated noise

2.1 Normal test

Measured Value (dB)
15.6

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Measured value (dB)
A - weight	14.2
C - weight	20.5
Flat	26.0

3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
125	-0.1	-0.1	-0.1	± 1.5
1000	0.0	0.0	0.0	± 1.0
8000	2.0	2.0	2.1	±5.0

เอกสารนี้เป็นความลับ

Cert. No. : ACL24160
Job No. : VC67AC0071
Pages : 5 of 8

4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	-0.1	-0.1	-0.1	±2.0
125	0.0	0.0	-0.1	±1.5
250	0.0	0.0	-0.1	±1.5
500	0.0	0.0	-0.1	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.0	0.0	±2.0
4000	0.0	0.0	0.0	±3.0
8000	0.0	0.0	0.0	±5.0

5. Frequency and time weightings at 1 kHz

5.1 Frequency weightings at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.2
C - weight	94.0	94.0	0.0	± 0.2
Flat	94.0	94.0	0.0	± 0.2

5.2 Time weighting at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	94.0	94.0	0.0	± 0.1
Slow	94.0	94.0	0.0	± 0.1
Leq	94.0	94.0	0.0	± 0.1

6. Long - term stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	

เอกสารไม่ควบคุม

SITHIPORN ASSOCIATES CO., LTD.

CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand
Tel. +66 2433 8331 Email : calibration@sithiporn.com

SITHIPORN
associates



Cert. No. : ACL24160

Job No. : VC67AC0071

Pages : 6 of 8

7. Level linearity on the reference level range

Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
137.0	137.1	0.1	± 1.1
136.0	136.1	0.1	± 1.1
135.0	135.1	0.1	± 1.1
134.0	134.1	0.1	± 1.1
133.0	133.0	0.0	± 1.1
132.0	132.0	0.0	± 1.1
131.0	131.0	0.0	± 1.1
129.0	129.1	0.1	± 1.1
124.0	124.0	0.0	± 1.1
119.0	119.1	0.1	± 1.1
114.0	114.1	0.1	± 1.1
109.0	109.1	0.1	± 1.1
104.0	104.1	0.1	± 1.1
99.0	99.1	0.1	± 1.1
94.0	94.0	0.0	± 1.1
89.0	89.0	0.0	± 1.1
84.0	84.0	0.0	± 1.1
79.0	79.0	0.0	± 1.1
74.0	74.0	0.0	± 1.1
69.0	69.0	0.0	± 1.1
64.0	64.0	0.0	± 1.1
59.0	59.0	0.0	± 1.1
54.0	54.0	0.0	± 1.1
49.0	49.0	0.0	± 1.1
44.0	44.0	0.0	± 1.1
39.0	39.0	0.0	± 1.1
34.0	34.0	0.0	± 1.1
30.0	30.0	0.0	± 1.1
29.0	29.0	0.0	± 1.1
28.0	28.1	0.1	± 1.1
27.0	27.1	0.1	± 1.1
26.0	26.2	0.2	± 1.1
25.0	25.2	0.2	± 1.1

เอกสารนี้เป็นความลับ

Cert. No. : ACL24160
Job No. : VC67AC0071
Pages : 7 of 8

8. Level linearity including the level range control

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Auto	94.0	94.0	0.0	±1.1

9. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Cycle	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.0	0.0	±1.0
Slow	2	8	108.0	108.0	0.0	1.5 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
SEL	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.0	0.0	±1.0

10. Peak C sound level

Number of cycle in test signal	Anticipated Value (dB)	Measured Value, Lcpeak (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	±3.0
One	136.4	136.4	0.0	±3.0

Number of cycle in test signal	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	±2.0
Positive half cycle	135.4	135.1	-0.3	±2.0
Negative half cycle	135.4	135.1	-0.3	±2.0

SITHIPORN ASSOCIATES CO., LTD.

CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand
Tel. +66 2433 8331 Email : calibration@sithiporn.com

SITHIPORN
associates



Cert. No. : ACL24160

Job No. : VC67AC0071

Pages : 8 of 8

11. Overload indication

Measured value (dB)		Deviated Value (dB)	Acceptance Limits (dB)
Positive one-half cycle	Negative one-half cycle		
89.6	89.5	-0.1	±1.5

12. High level stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor $k = 2$
or any value following calculation, providing a level of confidence of approximately 95 %

————— End of Calibration Certificate —————

เอกสารไม่ควบคุม



Certificate of Calibration

Customer

Name : UNITED ANALYST AND ENGINEERING
CONSULTANT CO.,LTD.
Address : 81 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Prakanong,
Bangkok 10260

Certificate No : 24-TPM-047

Request No : Req-2023-2686

Page : 1/2

Unit Under Calibration Details

Calibration Parameter	: Temperature	Range Calibration	: 20 °C to 60 °C
Instrument Name	: Thermal Environment Monitor	Type of Sensor	: RTD
Manufacturer	: TSI QUEST	Sensor Diameter (mm)	: 4.5
Model	: QT-34	Calibration Position (mm)	: 67.5
Serial Number	: TEG100075	Instrument Status	: Used
Resolution	: 0.1 °C		
ID Number	: UAE.EMA2.056/2552		

Calibration Environment and Details

Temperature : 23 °C ± 3 °C
Humidity : 55 %RH ± 15 %RH
Received Date : 21 December 2023
Calibrated Date : 23 January 2024
Calibration Procedure : In-house method CP-TPM-01 by Comparison with Standard Thermometer.

Reference Standard : Digital Thermometer with Sensor, Manufacturer: GINGO/GINGO, Model: GT11/ RTD100, SN:
08000057, ID: 02-TPM Which was calibrated on 27 Febuary 2023, Calibration Certificate No. : QR23-
0494

Traceability : This Certificate is traceable to SI Unit through Quality Reborn Co., Ltd., NSC-ONSC Accreditation No.:
Calibration 0292

Note

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor $k=2$, providing a level of confidence approximately 95 %.

Approved By :



Technical Manager

Issue Date :

23 January 2024

Calibration Note

UUC Adjustment : Not Adjust

Certificate No : 24-TPM-047

Request No : Req-2023-2686

Page : 2/2

Result of Calibration :

UUC Sensor	Standard Temperature (°C)	UUC Reading (°C)	Correction (°C)	Uncertainty (± °C)
WET	20.031	20.3	- 0.3	0.13
	25.032	25.3	- 0.3	0.13
	30.033	30.3	- 0.3	0.13
	35.037	35.3	- 0.3	0.13
	40.039	40.3	- 0.3	0.13
	45.040	45.3	- 0.3	0.13
	50.043	50.3	- 0.3	0.13
	60.046	60.3	- 0.3	0.13
DRY	20.031	20.2	- 0.2	0.13
	25.033	25.2	- 0.2	0.13
	30.035	30.2	- 0.2	0.13
	35.035	35.2	- 0.2	0.13
	40.038	40.2	- 0.2	0.13
	45.042	45.2	- 0.2	0.13
	50.042	50.2	- 0.2	0.13
	60.046	60.2	- 0.2	0.13
GLOBE	20.032	20.2	- 0.2	0.13
	25.033	25.2	- 0.2	0.13
	30.035	30.2	- 0.2	0.13
	35.037	35.2	- 0.2	0.13
	40.037	40.2	- 0.2	0.13
	45.039	45.2	- 0.2	0.13
	50.044	50.2	- 0.2	0.13
	60.046	60.2	- 0.2	0.13

End of Certificate

Calibrated By :





Certificate of Calibration

Customer

Name : UNITED ANALYST AND ENGINEERING
CONSULTANT CO.,LTD.
Address : 81 Soi Udomsuk 41, Sukhumvit Road, Bangchak,
Prakanong, Bangkok 10260

Certificate No : 24-TPM-152

Request No : Req-2024-0542

Page : 1/2

Unit Under Calibration Details

Calibration Parameter : Temperature
Instrument Name : Thermal Environment Monitor
Manufacturer : TSI QUEST
Model : QT-32
Serial Number : TPQ020025
Resolution : 0.1 °C
ID Number : UAE.EFM.008/2559

Range Calibration : 20 °C to 60 °C
Type of Sensor : RTD
Sensor Diameter (mm) : 4.5
Calibration Position (mm) : 67.5
Instrument Status : Used

Calibration Environment and Details

Temperature : 23 °C ± 3 °C
Humidity : 55 %RH ± 15 %RH
Received Date : 5 March 2024
Calibrated Date : 21 March 2024

Calibration Procedure : In-house method CP-TPM-01 by Comparison with Standard Thermometer.

Reference Standard : Digital Thermometer with Sensor, Manufacturer: GINGO/GINGO, Model: GT11/RTD100, SN: 12000077, ID: AR-TPM Which was calibrated on 27 October 2023, Calibration Certificate No. : QR23-2574

Traceability : This Certificate is traceable to SI Unit through Quality Reborn Co., Ltd., NSC-ONSC Accreditation No.: Calibration 0292

Note

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor $k=2$, providing a level of confidence approximately 95 %.

Approved By :



Technical Manager

Issue Date :

21 March 2024



Calibration Note

UUC Adjustment : Not Adjust

Certificate No : 24-TPM-152

Request No : Req-2024-0542

Page : 2/2

Result of Calibration :

UUC Sensor	Standard Temperature (°C)	UUC Reading (°C)	Correction (°C)	Uncertainty (± °C)
WET	20.030	20.1	- 0.1	0.13
	25.033	25.1	- 0.1	0.13
	30.035	30.1	- 0.1	0.13
	35.036	35.1	- 0.1	0.13
	40.038	40.2	- 0.2	0.13
	45.041	45.2	- 0.2	0.13
	50.044	50.2	- 0.2	0.13
	60.047	60.2	- 0.2	0.13
DRY	20.031	20.0	0.0	0.13
	25.033	25.0	0.0	0.13
	30.034	30.0	0.0	0.13
	35.036	35.0	0.0	0.13
	40.038	40.1	- 0.1	0.13
	45.039	45.1	- 0.1	0.13
	50.043	50.1	- 0.1	0.13
	60.047	60.1	- 0.1	0.13
GLOBE	20.032	20.1	- 0.1	0.13
	25.033	25.1	- 0.1	0.13
	30.034	30.1	- 0.1	0.13
	35.037	35.1	- 0.1	0.13
	40.038	40.1	- 0.1	0.13
	45.041	45.2	- 0.2	0.13
	50.044	50.2	- 0.2	0.13
	60.048	60.2	- 0.2	0.13

End of Certificate

Calibrated By :



Certificate of Calibration

Customer

Name : UNITED ANALYST AND ENGINEERING
CONSULTANT CO.,LTD.
Address : 81 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Prakanong,
Bangkok 10260

Certificate No : 24-TPM-043

Request No : Req-2023-2688

Page : 1/2

Unit Under Calibration Details

Calibration Parameter	: Temperature	Range Calibration	: 20 °C to 60 °C
Instrument Name	: Thermal Environment Monitor	Type of Sensor	: RTD
Manufacturer	: TSI QUEST	Sensor Diameter (mm)	: 4.5
Model	: QT-32	Calibration Position (mm)	: 67.5
Serial Number	: TPT060013	Instrument Status	: Used
Resolution	: 0.1 °C		
ID Number	: UAE.EFM.220/2562		

Calibration Environment and Details

Temperature : 23 °C ± 3 °C
Humidity : 55 %RH ± 15 %RH
Received Date : 21 December 2023
Calibrated Date : 23 January 2024
Calibration Procedure : In-house method CP-TPM-01 by Comparison with Standard Thermometer.


Reference Standard : Digital Thermometer with Sensor, Manufacturer: GINGO/GINGO, Model: GT11/ RTD100, SN:
08000057, ID: 02-TPM Which was calibrated on 27 Febuary 2023, Calibration Certificate No. : QR23-
0494

Traceability : This Certificate is traceable to SI Unit through Quality Reborn Co., Ltd., NSC-ONSC Accreditation No.:
Calibration 0292

Note

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor $k=2$, providing a level of confidence approximately 95 %.

Approved By :



Technical Manager

Issue Date :

23 January 2024

Calibration Note

UUC Adjustment : Not Adjust

Certificate No : 24-TPM-049

Request No : Req-2023-2691

Page : 2/2

Result of Calibration :

UUC Sensor	Standard Temperature (°C)	UUC Reading (°C)	Correction (°C)	Uncertainty (± °C)
WET	20.033	20.1	- 0.1	0.13
	25.033	25.1	- 0.1	0.13
	30.035	30.1	- 0.1	0.13
	35.036	35.1	- 0.1	0.13
	40.039	40.2	- 0.2	0.13
	45.040	45.2	- 0.2	0.13
	50.043	50.2	- 0.2	0.13
	60.047	60.2	- 0.2	0.13
DRY	20.031	20.2	- 0.2	0.13
	25.032	25.2	- 0.2	0.13
	30.035	30.2	- 0.2	0.13
	35.036	35.2	- 0.2	0.13
	40.038	40.3	- 0.3	0.13
	45.040	45.3	- 0.3	0.13
	50.042	50.3	- 0.3	0.13
	60.052	60.3	- 0.2	0.13
GLOBE	20.032	20.1	- 0.1	0.13
	25.032	25.1	- 0.1	0.13
	30.035	30.1	- 0.1	0.13
	35.035	35.1	- 0.1	0.13
	40.039	40.2	- 0.2	0.13
	45.040	45.1	- 0.1	0.13
	50.044	50.1	- 0.1	0.13
	60.045	60.1	- 0.1	0.13

End of Certificate

Calibrated By :



Certificate of Calibration

Customer

Name : UNITED ANALYST AND ENGINEERING CONSULTANT
CO.,LTD.
Address : 81 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Prakanong,
Bangkok 10260

Certificate No : 24-LXM-051

Request No : Req-2024-0183

Page : 1/2

Unit Under Calibration Details

Instrument Name : Light Meter
Manufacturer : EXTECH
Model : 407026
Serial Number : A052267
Resolution : 1 lx
ID Number : UAE.EFM.175/2564

Range Calibration : 2000 , 20000 lx

Instrument Status : Used

Calibration Environment and Details

Temperature : $25\text{ }^{\circ}\text{C} \pm 2\text{ }^{\circ}\text{C}$
Humidity : $60\text{ \%RH} \pm 20\text{ \%RH}$
Received Date : 26 January 2024
Calibrated Date : 29 February 2024
Calibration Procedure : The measurement was done in accordance with CP-LXM-01

Reference Standard : Photometer and Illuminance Sensor, Serial No.: 30662/2, 30592/2, which was calibrated on 31 October 2023,
Certificate No.: TP-1045-23

Traceability : This Certificate is traceable to International System of Unit (SI) Unit through National Institute of
Metrology (Thailand)

Note

The reported uncertainty is based on a standard uncertainty multiplied by the Coverage Factor $k = 2$, providing a level of confidence approximately 95 %.

Approved By :

Calibration Engineer Supervisor

Issue Date :

13 May 2024

เอกสารไม่ควบคุม

Calibration Note

UUC Adjustment : Zero adjustment before use

Certificate No : 24-LXM-051

Request No : Req-2024-0183

Page : 2/2

Result of Calibration :

UUC Range (lx)	Standard (lx)	UUC Reading (lx)	Correction (lx)	Uncertainty (\pm lx)
2000	*0	0	0	0.0058
	50	50	0	2.2 % of Reading
	100	101	-1	2.2 % of Reading
	200	201	-1	2.2 % of Reading
	300	303	-3	2.2 % of Reading
	400	402	-2	2.2 % of Reading
	600	602	-2	2.2 % of Reading
	800	803	-3	2.2 % of Reading
	1000	1004	-4	2.2 % of Reading
	1200	1203	-3	2.2 % of Reading
	1400	1405	-5	2.2 % of Reading
	1600	1605	-5	2.2 % of Reading
	1800	1809	-9	2.2 % of Reading
	2000	1990	10	2.2 % of Reading
20000	3000	2980	20	2.2 % of Reading
	4000	3970	30	2.2 % of Reading
	5000	4950	50	2.2 % of Reading

* Indicates non accredited

End of Certificate

Calibrated By :



เอกสารไม่ควบคุม

ภาคผนวก จ

ผลการควบคุมคุณภาพในการเก็บและตรวจวิเคราะห์ตัวอย่าง

RESULTS OF QUALITY ASSURANCE AND QUALITY CONTROL IN THE LABORATORY OF WASTEWATER FOR PTTLNG COMPANY LIMITED
PROJECT : AUDIT MITIGATION AND ENVIRONMENTAL MONITORING MEASURES DURING PTTLNG RECEIVING TERMINAL OPERATION

SAMLING DATE : DECEMBER 25, 2024

PARAMETER	UNIT	DETECTION LIMIT	METHOD BLANK	T24BE374-0003			LABORATORY FORTIFIED BLANK (LFB)	
				DUPLICATE			NOMINAL	MEASURED
				1	2	RPD		
BIOCHEMICAL OXYGEN DEMAND	mg/L	2.0	<2.0	68.2	63.0	7.93	198.0	206
ACCEPTABLE LIMIT						≤20	198.0±30.5 (167.5 - 228.5)	

พารามิเตอร์	หน่วย	DETECTION LIMIT	METHOD BLANK	T24BE401-0001			QC STANDARD		
				DUPLICATE			NOMINAL	MEASURED	%RECOVERY
				1	2	RPD			
TOTAL SUSPENDED SOLIDS	mg/L	5.0	< 2.0	195	193	1.03	100	95.8	95.8
ACCEPTABLE LIMIT						≤10			90-110

PARAMETER	UNIT	DETECTION LIMIT	METHOD BLANK	T24BE400-0002			LABORATORY FORTIFIED BLANK (LFB)		
				DUPLICATE			NOMINAL	MEASURED	%RECOVERY
				1	2	RPD			
TOTAL DISSOLVED SOLIDS	mg/L	25	< 25	514	504	1.96	50	51	102
ACCEPTABLE LIMIT						≤ 10			90-110

PARAMETER	UNIT	DETECTION LIMIT	METHOD BLANK	T24BE377-0002			LABORATORY FORTIFIED BLANK (LFB)		
				DUPLICATE			NOMINAL	MEASURED	%RECOVERY
				1	2	RPD			
CHEMICAL OXYGEN DEMAND	mg/L	25.0	<25.0	50.6	47.4	6.53	50.0	47.4	94.8
ACCEPTABLE LIMIT						≤ 10			90-110

PARAMETER	UNIT	DETECTION LIMIT	METHOD BLANK	T24BE385-0002			LABORATORY FORTIFIED BLANK (LFB)		
				DUPLICATE			NOMINAL	MEASURED	%RECOVERY
				1	2	RPD			
TOTAL KJELDAHL NITROGEN	mg/L	1.5	<1.5	42.7	42.5	0.47	40.0	40.0	100
ACCEPTABLE LIMIT						≤ 10			90-110

PARAMETER	UNIT	DETECTION LIMIT	METHOD BLANK	LABORATORY FORTIFIED BLANK (LFB)		
				NOMINAL	MEASURED	%RECOVERY
FAT, OIL AND GREASE	mg/L	1.0	<3	40	35.3	88.3
ACCEPTABLE LIMIT						75-110

PARAMETER	UNIT	DETECTION LIMIT	METHOD BLANK	INITIAL CALIBRATION VERIFICATION (ICV)			LABORATORY FORTIFIED BLANK (LFB)			T24BE252-0003		
				NOMINAL	MEASURED	%RECOVERY	NOMINAL	MEASURED	%RECOVERY	RESULT		
										DUPLICATE		
										1	2	RPD
LEAD	mg/L Pb	0.020	< 0.020	0.700	0.714	102	0.700	0.668	95.4	< 0.020	< 0.020	-
CADMIUM	mg/L Cd	0.005	< 0.005	0.300	0.312	104	0.300	0.294	98.0	< 0.005	< 0.005	-
ACCEPTABLE LIMIT						90 ± 10%			85 ± 11%			≤ 10%

PARAMETER	UNIT	T24BE252-0003				LABORATORY FORTIFIED BLANK (LFB)			CONTINUING CALIBRATION VERIFICATION (CCV)		
		RESULT									
		LABORATORY FORTIFIED MATRIX (LFM)				NOMINAL	MEASURED	%RECOVERY	NOMINAL	MEASURED	%RECOVERY
		SAMPLE	NOMNAL	MEASURED	%RECOVERY						
LEAD	mg/L Pb	< 0.020	0.700	0.661	94.4	0.700	0.662	94.6	0.700	0.669	95.6
CADMIUM	mg/L Cd	< 0.005	0.300	0.274	91.3	0.300	0.293	97.7	0.300	0.294	98.0
ACCEPTABLE LIMIT					85 - 115%			85 - 115%			90 - 110%

PARAMETER	UNIT	DETECTION LIMIT	METHOD BLANK	INITIAL CALIBRATION VERIFICATION (ICV)			LABORATORY FORTIFIED BLANK (LFB)			T25AA016-0007		
				NOMINAL	MEASURED	%RECOVERY	NOMINAL	MEASURED	%RECOVERY	RESULT		
										DUPLICATE		
										1	2	RPD
MERCURY	mg/L Hg	0.0005	< 0.0005	0.0060	0.0060	100	0.0060	0.0057	95.0	0.0014	0.0014	0
ACCEPTABLE LIMIT						90 ± 10%			85 ± 11%			≤ 10%

PARAMETER	UNIT	T25AA016-0007				LABORATORY FORTIFIED BLANK (LFB)			CONTINUING CALIBRATION VERIFICATION (CCV)		
		RESULT									
		LABORATORY FORTIFIED MATRIX (LFM)				NOMINAL	MEASURED	%RECOVERY	NOMINAL	MEASURED	%RECOVERY
		SAMPLE	NOMNAL	MEASURED	%RECOVERY						
MERCURY	mg/L Hg	< 0.0005	0.0060	0.0061	102	0.0060	0.0062	103	0.0060	0.0062	103
ACCEPTABLE LIMIT					85 - 115%			85 - 115%			90 - 110%

ภาคผนวก ฉ

หนังสือขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์

วันที่ 3 เดือน ธันวาคม พ.ศ. 2567

ข้าพเจ้า ☐ ผู้รับใบอนุญาตประกอบกิจการโรงงาน

☒ บริษัท/ทางหันส่วนจำกัด / บริษัท ยูนิตี้ แอวนาลิสต์ แอนด์ เอ็นจิเนียริ่ง คอนซัลแตนท์ จำกัด

กองวิจัยและฝึกอบรมกักกันโรค
วันที่ ๒๕/๕/๕๔

Due to the fact that the data are not available for the entire country, the results are not representative of the entire country.

คุณชัชวาลย์ แสนบุญชู

สถานที่ตั้งห้องปฏิบัติการ

เลขที่ 3 หมู่ที่ - ต.รอก/ซอย อุดมสุข 41 ถนน สานนิต

ตำบล/แขวง _____ อำเภอ/เขต _____ พระโขนง _____ จังหวัด กรุงเทพมหานคร _____

รหัสไปรษณีย์ 10260 โทรศัพท์ 02 763 2828 E-mail lab.support3@uaeconsultant.co.th

เลขทะเบียนหนังสือปฏิบัติการ ๖-145

ได้รับทราบ ประกาศกรมโรงงานอุตสาหกรรม เรื่อง หอ้งปฏิบัติการวิเคราะห์เอกชน พ.ศ. 2566 โดยตลอดแล้ว และยินยอมปฏิบัติตามประกาศฯ ทุกประการ และได้แนบเอกสารต่างๆ ตามรายการเอกสารประกอบการพิจารณา (แบบ ปอ.1-1) มาพร้อมนี้

การดำเนินการ	จำนวนสารมลพิษ					
	น้ำเสีย/น้ำทิ้ง (รายการ)	น้ำใต้ดิน (รายการ)	อากาศ (รายการ)	สิ่งปฏิกูลหรือ วัสดุที่ไม่ใช้ แล้ว(รายการ)	ดิน (รายการ)	รวมทั้งสิ้น (รายการ)
<input type="checkbox"/> ขออนุญาตขุดลอกหรือ ขุดลอก						
<input checked="" type="checkbox"/> ต่ออายุขุดลอกหรือ ขุดลอก	46	126	25	35	126	358
<input type="checkbox"/> เปลี่ยนแปลงสารมลพิษที่ วิเคราะห์ <input type="radio"/> เพิ่มสารมลพิษ <input type="radio"/> ยกเลิกสารมลพิษ						
<input type="checkbox"/> เปลี่ยนแปลงบุคลากร <input type="radio"/> เพิ่มบุคลากร <input type="radio"/> ยกเลิกบุคลากร	จำนวน.....ราย (รายละเอียดตาม แบบ ปว.1) จำนวน.....ราย (รายละเอียดตาม แบบ ปว.1-1)					
<input type="checkbox"/> ยกเลิกขุดลอกหรือ ขุดลอก						
<input type="checkbox"/> อื่นๆ โปรดระบุ.....						

จึงเรียนมาเพื่อโปรดพิจารณา

0491 -

เทิดไท้บรรพบุรุษ

นักวิทยาศาสตร์ผู้เชี่ยวชาญ วิทยาลัยการแพทย์
ผู้อำนวยการกองวิจัยและพัฒนาระบบนิเวศวิทยา

UNITE
UNITED ANALYST AND ENGINEERING
CONSULTANT COMPANY LIMITED

ผู้มีอำนาจลงนามแทนนิติบุคคล
ประทับตรา (ถ้ามี)

ที่ UAE05831/2024

สำเนา

วันที่ 27 พฤศจิกายน พ.ศ. 2567

เรื่อง ขออนุญาตต่ออายุหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน

เรียน อธิบดีกรมโรงงานอุตสาหกรรม

สิ่งที่ส่งมาด้วย เอกสารประกอบการขออนุญาตต่ออายุหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน

ตามที่บริษัท ยูไนเต็ด แอนาไลสต์ แอนด์ เอ็นจิเนียริง คอนซัลแตนท์ จำกัด ได้รับอนุญาต
จากกรมโรงงานอุตสาหกรรม ให้ขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน เลขทะเบียน ว-145 นั้น

ในการนี้บริษัทฯ มีความประสงค์ขออนุญาตต่ออายุหนังสือรับขึ้นทะเบียนห้องปฏิบัติการ
วิเคราะห์เอกชน โดยมีองค์ประกอบ ดังนี้

1. ผู้ควบคุมดูแลห้องปฏิบัติการวิเคราะห์ จำนวน 39 ราย
2. เจ้าหน้าที่ประจำห้องปฏิบัติการวิเคราะห์ จำนวน 142 ราย
3. สารมลพิษวิเคราะห์ในน้ำเสีย จำนวน 46 รายการ น้ำใต้ดิน จำนวน 126 รายการ
อากาศเสีย จำนวน 25 รายการ สิ่งปฏิกูลหรือวัสดุที่ไม่ใช้แล้ว จำนวน 35 รายการ และดิน
จำนวน 126 รายการ รวมทั้งสิ้น จำนวน 358 รายการ

ทั้งนี้บริษัทฯ ได้แนบเอกสารประกอบการขออนุญาตต่ออายุหนังสือรับขึ้นทะเบียนห้อง
ปฏิบัติการวิเคราะห์เอกชนดังสิ่งที่ส่งมาด้วย

จึงเรียนมาเพื่อโปรดพิจารณา

ขอแสดงความนับถือ

UAE
UNITED ANALYST AND ENGINEERING
CONSULTANT COMPANY LIMITED

UAE
UNITED ANALYST AND ENGINEERING
CONSULTANT COMPANY LIMITED

สำเนาถูกต้อง

3/12/67

ประกาศกรมโรงงานอุตสาหกรรม

เรื่อง ห้องปฏิบัติการวิเคราะห์เอกซน

พ.ศ. ๒๕๖๖

โดยที่เป็นการสมควรให้มีการปรับปรุง หลักเกณฑ์และวิธีการเกี่ยวกับการเป็นห้องปฏิบัติการวิเคราะห์เอกซนเพื่อประโยชน์ในการปฏิบัติตามข้อ ๓ ของประกาศกระทรวงอุตสาหกรรม เรื่อง กำหนดลักษณะของน้ำมันใช้แล้วที่ผ่านกระบวนการปรับปรุงคุณภาพและเชื้อเพลิงสังเคราะห์ที่จะนำมาใช้เป็นเชื้อเพลิงในเตาอุตสาหกรรมเพื่อทดแทนน้ำมันเตา พ.ศ. ๒๕๕๗ ข้อ ๑๒ ของประกาศกระทรวงอุตสาหกรรม เรื่อง การจัดทำรายงานชนิดและปริมาณสารมลพิษที่ระบายออกจากโรงงาน พ.ศ. ๒๕๕๘ ข้อ ๗ ของกฎกระทรวงควบคุมการปนเปื้อนในดินและน้ำใต้ดินภายในบริเวณโรงงาน พ.ศ. ๒๕๕๙ ข้อ ๔.๒ ของประกาศกรมโรงงานอุตสาหกรรม เรื่อง หลักเกณฑ์การให้ความเห็นชอบโรงงานที่ต้องมีระบบบำบัดน้ำเสียต้องติดตั้งเครื่องมือหรือเครื่องอุปกรณ์พิเศษและเครื่องมือหรือเครื่องอุปกรณ์ พ.ศ. ๒๕๕๐ ซึ่งแก้ไขเพิ่มเติมโดยประกาศกรมโรงงานอุตสาหกรรม เรื่อง หลักเกณฑ์การให้ความเห็นชอบโรงงานที่ต้องมีระบบบำบัดน้ำเสียต้องติดตั้งเครื่องมือหรือเครื่องอุปกรณ์พิเศษและเครื่องมือหรือเครื่องอุปกรณ์ (ฉบับที่ ๒) พ.ศ. ๒๕๖๕ ข้อ ๑๕ ของประกาศกระทรวงอุตสาหกรรม เรื่อง การจัดการสิ่งปฏิกูลหรือวัสดุที่ไม่ใช้แล้ว พ.ศ. ๒๕๖๖ และการตรวจวัดวิเคราะห์ค่าที่จำเป็นประกอบการพิจารณาดำเนินการตามพระราชบัญญัติโรงงาน พ.ศ. ๒๕๓๕ และที่แก้ไขเพิ่มเติม กรมโรงงานอุตสาหกรรม จึงออกประกาศไว้ ดังต่อไปนี้

ข้อ ๑ ประกาศนี้เรียกว่า “ประกาศกรมโรงงานอุตสาหกรรม เรื่อง ห้องปฏิบัติการวิเคราะห์เอกซน พ.ศ. ๒๕๖๖”

ข้อ ๒ ประกาศนี้ให้ใช้บังคับตั้งแต่วันถัดจากวันประกาศในราชกิจจานุเบกษาเป็นต้นไป

ข้อ ๓ ให้ยกเลิกระเบียบกรมโรงงานอุตสาหกรรมว่าด้วยการขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกซน พ.ศ. ๒๕๖๐

หมวด ๑

บททั่วไป

ข้อ ๔ ในประกาศนี้

“ห้องปฏิบัติการวิเคราะห์เอกซน” หมายความว่า ห้องปฏิบัติการวิเคราะห์ที่มีอาคารสถานที่ตั้งเหมาะสมเป็นการถาวรสำหรับการให้บริการตรวจวัดวิเคราะห์ทดสอบสารมลพิษที่กรมโรงงานอุตสาหกรรมกำหนดหรือเห็นชอบหรือรับรองเพื่อปฏิบัติตามที่พระราชบัญญัติโรงงาน พ.ศ. ๒๕๓๕ และที่แก้ไขเพิ่มเติมกำหนด ซึ่งห้องปฏิบัติการวิเคราะห์ตามข้อนี้ต้องมีชื่อห้องปฏิบัติการวิเคราะห์ขึ้นทะเบียนกับกรมโรงงานอุตสาหกรรมหรือมหาวิทยาลัยในกำกับของรัฐ

UNITED ANALYST AND ENGINEERING
CONSULTANT COMPANY LIMITED

ดำเนินการถูกต้อง

“สารมลพิษ” หมายความว่า ตัวบ่งชี้คุณลักษณะของตัวอย่างหรือตัวกลางด้านสิ่งแวดล้อมตามที่กฎหมายกำหนด

“ผู้ควบคุมห้องปฏิบัติการวิเคราะห์เอกชน” หมายความว่า บุคลากรผู้ปฏิบัติงานประจำของห้องปฏิบัติการวิเคราะห์เอกชน ซึ่งเป็นผู้ดำเนินการวางแผน กำหนด ควบคุม เลือกใช้เทคนิคการวิเคราะห์ เครื่องมือ อุปกรณ์ ในการตรวจวัด วิเคราะห์ทดสอบให้เป็นไปตามกฎหมายและตามวิธีมาตรฐาน การเข้าร่วมทดสอบความชำนาญหรือการเปรียบเทียบผลระหว่างห้องปฏิบัติการ (ถ้ามี) การบริหารงานของห้องปฏิบัติการวิเคราะห์เอกชน ตามประกาศนี้ และลงนามรับรองรายงานผล

“เจ้าหน้าที่ห้องปฏิบัติการวิเคราะห์เอกชน” หมายความว่า บุคลากรผู้ปฏิบัติงานประจำของห้องปฏิบัติการวิเคราะห์เอกชน ซึ่งเป็นผู้ดำเนินการตรวจวัด เก็บตัวอย่าง และวิเคราะห์ทดสอบสารมลพิษ การจัดการตัวอย่าง การควบคุมคุณภาพ การบันทึกข้อมูลผลการตรวจวัด เก็บตัวอย่าง และวิเคราะห์ทดสอบสารมลพิษ

“เลขทะเบียน” หมายความว่า กลุ่มเลขและหรือตัวอักษรที่กรมโรงงานอุตสาหกรรมกำหนดขึ้นเพื่อแสดงว่าได้มีการขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน

“รายงานผล” หมายความว่า รายงานผลการตรวจวัดวิเคราะห์ทดสอบสารมลพิษของห้องปฏิบัติการวิเคราะห์เอกชน

หมวด ๒

ห้องปฏิบัติการวิเคราะห์เอกชน

ข้อ ๕ ห้องปฏิบัติการวิเคราะห์เอกชนที่กรมโรงงานอุตสาหกรรมกำหนด หรือเห็นชอบหรือรับรอง ตามกฎหมายว่าด้วยโรงงาน ต้องขึ้นทะเบียนต่อกรมโรงงานอุตสาหกรรม

ข้อ ๖ ห้องปฏิบัติการวิเคราะห์ที่สามารถขึ้นทะเบียนเป็นห้องปฏิบัติการวิเคราะห์เอกชนตามข้อ ๕ ได้ต้องมีคุณสมบัติ มีบุคลากรและการดำเนินการ ดังนี้

๖.๑ เป็นนิติบุคคลซึ่งเป็นผู้ประกอบกิจการโรงงานตามกฎหมายว่าด้วยโรงงาน หรือเป็นนิติบุคคลที่มีวัตถุประสงค์เพื่อรับจ้างหรือให้บริการที่เกี่ยวข้องกับการตรวจวัด เก็บตัวอย่าง และวิเคราะห์ทดสอบสารมลพิษ

๖.๒ มีผู้ควบคุมห้องปฏิบัติการวิเคราะห์เอกชน ซึ่งต้องมีคุณสมบัติและการดำเนินการ ดังนี้

๖.๒.๑ มีคุณวุฒิและมีประสบการณ์อย่างใดอย่างหนึ่ง ดังต่อไปนี้

(ก) สำเร็จการศึกษาในระดับไม่ต่ำกว่าปริญญาตรี ทางวิทยาศาสตร์ วิศวกรรมศาสตร์ ศึกษาศาสตร์ หรือครุศาสตร์ โดยมีสาขาวิชาตามรายละเอียดในภาคผนวก ก และมีประสบการณ์วิเคราะห์สารมลพิษในห้องปฏิบัติการวิเคราะห์เป็นระยะเวลา

(ข) สำเร็จการศึกษาในระดับไม่ต่ำกว่าปริญญาตรีทางวิทยาศาสตร์ วิศวกรรมศาสตร์ ศาสตร์ หรือครุศาสตร์ ในสาขาอื่นนอกเหนือจากสาขาวิชาตามรายละเอียดในภาคผนวก ก และมีวิชาเรียนทางด้านเคมีหรือวิชาเรียนที่เกี่ยวข้องกับการตรวจวัด เก็บตัวอย่าง และวิเคราะห์ทดสอบสารมลพิษไม่น้อยกว่า ๑๕ หน่วยกิต และมีประสบการณ์วิเคราะห์สารมลพิษในห้องปฏิบัติการวิเคราะห์เป็นระยะเวลาไม่น้อยกว่า ๕ ปี

(ค) เคยเป็นเจ้าหน้าที่ห้องปฏิบัติการวิเคราะห์เอกชนซึ่งกรมโรงงานอุตสาหกรรมขึ้นทะเบียนหรือให้การรับรองมาแล้วไม่น้อยกว่า ๑๐ ปี

(ง) คุณสมบัติอื่นนอกเหนือจาก (ก) (ข) หรือ (ค) ตามที่กรมโรงงานอุตสาหกรรมเห็นชอบ

๖.๒.๒ ผ่านการฝึกอบรมด้านการควบคุมคุณภาพการวิเคราะห์ทดสอบ และด้านข้อกำหนดทั่วไปว่าด้วยความสามารถของห้องปฏิบัติการทดสอบและห้องปฏิบัติการสอบเทียบ มอก. ๑๗๐๒๕ (ISO/IEC 17025) จากหน่วยงานและรูปแบบการฝึกอบรมตามรายละเอียดในภาคผนวก ข

๖.๒.๓ กรณีที่มีผู้ใช้ที่มีคุณสมบัติตาม ๖.๒.๑ และ ๖.๒.๒ จะต้องเป็นผู้มีใบอนุญาตประกอบวิชาชีพวิทยาศาสตร์และเทคโนโลยีควบคุม สาขาการวิเคราะห์มลพิษ สิ่งแวดล้อมด้านวิทยาศาสตร์และการควบคุมมลพิษ ประเภทผู้เชี่ยวชาญเฉพาะด้านติดตามตรวจสอบมาตรการด้านสิ่งแวดล้อม หรือผู้ที่ได้รับการรับรองความสามารถบุคลากรตามมาตรฐาน ISO/IEC 17024 สาขาการควบคุมคุณภาพการวิเคราะห์ด้านสิ่งแวดล้อม เท่านั้น

๖.๒.๔ ต้องปฏิบัติงานประจำห้องปฏิบัติการวิเคราะห์ที่ขอขึ้นทะเบียนเพียงแห่งเดียวเท่านั้น

๖.๓ มีเจ้าหน้าที่ห้องปฏิบัติการวิเคราะห์เอกชน ซึ่งต้องมีคุณสมบัติและการดำเนินการ ดังนี้

๖.๓.๑ มีคุณสมบัติหรือมีประสบการณ์อย่างใดอย่างหนึ่ง ดังต่อไปนี้

(ก) สำเร็จการศึกษาในระดับไม่ต่ำกว่าปริญญาตรี ทางวิทยาศาสตร์ วิศวกรรมศาสตร์ ศาสตร์ หรือครุศาสตร์ โดยมีสาขาวิชาตามรายละเอียดในภาคผนวก ก

(ข) สำเร็จการศึกษาในระดับไม่ต่ำกว่าปริญญาตรีทางวิทยาศาสตร์ วิศวกรรมศาสตร์ ศาสตร์ หรือครุศาสตร์ ในสาขาอื่นนอกเหนือจากสาขาวิชาตามรายละเอียดในภาคผนวก ก และมีวิชาเรียนทางด้านเคมีหรือวิชาเรียนที่เกี่ยวข้องกับการตรวจวัด เก็บตัวอย่าง และวิเคราะห์ทดสอบสารมลพิษไม่น้อยกว่า ๑๕ หน่วยกิต

(ค) สำเร็จปริญญาตรีด้านเคมีปฏิบัติ ประกาศนียบัตรวิชาชีพเคมีเทคนิค เหมืองอุตสาหกรรม เคมีปฏิบัติการหรือปิโตรเคมี

(ง) มัธยมศึกษาปีที่ ๖ หรือเทียบเท่าที่มีวิชาเรียนเคมี และมีประสบการณ์วิเคราะห์สารมลพิษในห้องปฏิบัติการเป็นระยะเวลาไม่น้อยกว่า ๑๐ ปี

๖.๓.๒ ผ่านการฝึกอบรมด้านการควบคุมคุณภาพการวิเคราะห์ทดสอบและด้านข้อกำหนดทั่วไปว่าด้วยความสามารถของห้องปฏิบัติการทดสอบและห้องปฏิบัติการสอบเทียบ มอก. ๑๗๐๒๕ (ISO/IEC 17025) จากหน่วยงานและรูปแบบการฝึกอบรมตามรายละเอียดในภาคผนวก ข

๖.๓.๓ ต้องปฏิบัติงานประจำห้องปฏิบัติการวิเคราะห์ที่ขอขึ้นทะเบียนเพียงแห่งเดียวเท่านั้น

๖.๔ มีวิธีปฏิบัติการตรวจวัด การเก็บตัวอย่าง และการวิเคราะห์ทดสอบตามหมวด ๓ รวมทั้งมีการควบคุมคุณภาพการวิเคราะห์ตามกฎหมายหรือตามที่มีการยอมรับและเชื่อถือได้

๖.๕ มีการบริหารจัดการด้านความปลอดภัยภายในห้องปฏิบัติการที่เหมาะสม เช่น อุปกรณ์ป้องกันส่วนบุคคล ระบบระบายอากาศเสีย ตู้ดูดควัน อุปกรณ์ชะล้างร่างกายแบบฉุกเฉิน เครื่องมือปฐมพยาบาล ระบบหรืออุปกรณ์ดับเพลิง เป็นต้น

๖.๖ มีการจัดการสารเคมี และการจัดการของเสียที่เกิดจากการตรวจวัดวิเคราะห์ทดสอบ

๖.๗ มีการประเมินสมรรถนะและเฝ้าระวังบุคลากร เพื่อให้มั่นใจว่า บุคลากรมีความสามารถดำเนินกิจกรรมของห้องปฏิบัติการในส่วนที่ตนรับผิดชอบและมีความสามารถประเมินความเียงเบนที่มีนัยสำคัญ

หมวด ๓

การตรวจวัด การเก็บตัวอย่าง และการวิเคราะห์ทดสอบ

ข้อ ๗ ห้องปฏิบัติการวิเคราะห์เอกชนที่ได้รับการขึ้นทะเบียนจากกรมโรงงานอุตสาหกรรมตามประกาศนี้ ต้องทำการตรวจวัด เก็บตัวอย่าง และวิเคราะห์ทดสอบสารมลพิษ โดยใช้วิธีการ เครื่องมือและอุปกรณ์ ดังต่อไปนี้

๗.๑ การตรวจวัด การเก็บตัวอย่าง และการวิเคราะห์ทดสอบสารมลพิษในน้ำ กำหนดให้ใช้วิธีการ เครื่องมือและอุปกรณ์ตาม Standard Methods for the Examination of Water and Wastewater ซึ่ง American Public Health Association, American Water Works Association และ Water Environment Federation ของสหรัฐอเมริกา ร่วมกันกำหนด หรือตามคู่มือวิเคราะห์น้ำและน้ำเสียของสมาคมวิศวกรรมสิ่งแวดล้อมแห่งประเทศไทย หรือตามวิธีการที่กฎหมายกำหนด หรือตามวิธีการอื่นที่กรมโรงงานอุตสาหกรรมเห็นชอบ

๗.๒ การตรวจวัด การเก็บตัวอย่าง และการวิเคราะห์ทดสอบสารมลพิษในอากาศ กำหนดให้ใช้วิธีการ เครื่องมือและอุปกรณ์ตาม United States Environmental Protection Agency หรือตามวิธีการที่กฎหมายกำหนด หรือตามวิธีการอื่นที่กรมโรงงานอุตสาหกรรมเห็นชอบ

๗.๓ การเก็บตัวอย่างและการวิเคราะห์ทดสอบสารมลพิษในสิ่งปฏิกูลหรือวัสดุที่ไม่ใช้แล้ว กำหนดให้ใช้วิธีการ เครื่องมือและอุปกรณ์ตาม Test Methods For Evaluating Solid Waste : Physical/Chemical Methods (SW-846) ของ United States Environmental Protection Agency หรือวิธีของ American Society for Testing and Materials (ASTM) หรือตามวิธีการที่กฎหมายกำหนด หรือตามวิธีการอื่นที่กรมโรงงานอุตสาหกรรมเห็นชอบ

๗.๔ การเก็บตัวอย่าง และการวิเคราะห์ทดสอบสารมลพิษในดิน กำหนดให้ใช้วิธีการ เครื่องมือและอุปกรณ์ตาม Test Methods For Evaluating Solid Waste : Physical/Chemical Methods (SW-846) ของ United States Environmental Protection Agency หรือตามวิธีการที่กฎหมายกำหนด หรือตามวิธีการอื่นที่กรมโรงงานอุตสาหกรรมเห็นชอบ

๗.๕ การเก็บตัวอย่าง และการวิเคราะห์ทดสอบสารมลพิษในน้ำใต้ดิน กำหนดให้ใช้วิธีการ เครื่องมือและอุปกรณ์ตาม Standard Methods for the Examination of Water and Wastewater ซึ่ง American Public Health Association, American Water Works Association และ Water Environment Federation ของสหรัฐอเมริกา ร่วมกันกำหนด หรือตามวิธีการที่กฎหมายกำหนด หรือตามวิธีการอื่นที่กรมโรงงานอุตสาหกรรมเห็นชอบ

๗.๖ การวิเคราะห์ทดสอบตาม ๗.๑, ๗.๓, ๗.๔ และ ๗.๕ สำหรับตรวจวัดโลหะ สารฆ่าศัตรูพืชและสัตว์ สารอินทรีย์ระเหยง่าย ห้องปฏิบัติการวิเคราะห์ต้องแสดงช่วงความสามารถ (Range) แสดงค่าปริมาณต่ำสุดที่สามารถวัดได้ (LOD) ค่าปริมาณต่ำสุดที่สามารถวัดได้โดยมีความแม่นยำและความเที่ยง (LOQ) โดยทั้งหมดต้องเป็นไปตามหลักวิชาการและสอดคล้องกับค่ามาตรฐาน

หมวด ๔

การรับขึ้นทะเบียน และต่ออายุการรับขึ้นทะเบียน

ข้อ ๘ ห้องปฏิบัติการวิเคราะห์เอกชนที่มีคุณสมบัติมีบุคลากรและการดำเนินการตามหมวด ๒ ที่ประสงค์จะขึ้นทะเบียนต่อกรมโรงงานอุตสาหกรรม ให้ยื่นคำขอพร้อมเอกสารประกอบตามที่กำหนดในคำขอ

ข้อ ๙ กรมโรงงานอุตสาหกรรมจะตรวจสอบการดำเนินงาน ณ ห้องปฏิบัติการวิเคราะห์เอกชน หรือสถานที่ปฏิบัติงานในภาคสนาม เพื่อประกอบการพิจารณาคำขอ โดยให้บุคลากรตามข้อ ๖.๒ อำนวยความสะดวก ช่วยเหลือ ให้ข้อมูลหรือคำชี้แจง แก่พนักงานเจ้าหน้าที่หรือผู้ที่ได้รับมอบหมายจากกรมโรงงานอุตสาหกรรม

กรณีที่กรมโรงงานอุตสาหกรรมตรวจสอบและพิจารณาคำขอพร้อมคำชี้แจงแล้ว เห็นว่าผู้ยื่นคำขอมิคุณสมบัติ มีบุคลากรและการดำเนินการ ครบถ้วนตามหมวด ๒ ให้อธิบดีกรมโรงงานอุตสาหกรรมหรือผู้ซึ่งอธิบดีกรมโรงงานอุตสาหกรรมมอบหมาย รับขึ้นทะเบียน

ห้องปฏิบัติการวิเคราะห์เอกซเรย์ดังกล่าวภายใน ๖๐ วัน โดยการรับขึ้นทะเบียนให้มีการออกหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกซเรย์ เลขทะเบียน ผู้ควบคุมห้องปฏิบัติการวิเคราะห์เอกซเรย์ เจ้าหน้าที่ห้องปฏิบัติการวิเคราะห์เอกซเรย์ รวมทั้งชนิดสารมลพิษที่ได้รับขึ้นทะเบียน ให้กับผู้ยื่นคำขอ

การรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกซเรย์ตามวรรคสองให้มีอายุ ๔ ปี นับตั้งแต่วันที่ออกหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกซเรย์

ข้อ ๑๐ การรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกซเรย์ ตามข้อ ๙ ให้สามารถต่ออายุ การรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกซเรย์ได้คราวละ ๔ ปี โดยให้นับอายุต่อจากวันสิ้นอายุของการขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกซเรย์เดิมก่อนต่ออายุ

ข้อ ๑๑ การต่ออายุการรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกซเรย์ ให้ยื่นคำขอต่ออายุ พร้อมเอกสารหลักฐานประกอบตามที่กำหนดในคำขอและสรุปผลการดำเนินงานที่ผ่านมา ภายใน ๖๐ วัน ก่อนวันสิ้นอายุของการรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกซเรย์ และให้นำความในข้อ ๙ และข้อ ๑๐ มาบังคับใช้กับการพิจารณาคำขอต่ออายุโดยอนุโลม

เมื่อได้ยื่นคำขอต่ออายุตามเวลาที่กำหนดแล้ว ให้ถือว่าผู้ยื่นคำขอต่ออายุอยู่ในฐานะผู้ได้รับการขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกซเรย์ไปก่อนจนกว่ากรมโรงงานอุตสาหกรรมจะไม่ต่ออายุ การขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกซเรย์ให้

ในกรณีคำขอต่ออายุเพื่อทำการตรวจวัดและเก็บตัวอย่างสารมลพิษอากาศ ห้องปฏิบัติการ ต้องมีเอกสารข้อมูลการตรวจวัดและเก็บตัวอย่างที่มีพนักงานเจ้าหน้าที่หรือผู้ที่ได้รับมอบหมายจาก กรมโรงงานอุตสาหกรรมเข้าตรวจสอบการดำเนินงานในภาคสนามด้วย ไม่น้อยกว่า ๑ ครั้ง

กรณีที่ยื่นคำขอต่ออายุไม่ทันกำหนดระยะเวลาตามวรรคหนึ่ง ให้ดำเนินการเสมือนการยื่นคำขอ ขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกซเรย์ใหม่

ข้อ ๑๒ การตรวจติดตามผลการดำเนินงานของห้องปฏิบัติการ ให้ดำเนินการไม่น้อยกว่า ๑ ครั้ง

ข้อ ๑๓ ห้องปฏิบัติการวิเคราะห์เอกซเรย์ที่กรมโรงงานอุตสาหกรรมรับขึ้นทะเบียนแล้ว หากประสงค์ จะเปลี่ยนแปลงบุคลากรตามหมวด ๒ หรือเปลี่ยนแปลงชนิดสารมลพิษที่ได้รับขึ้นทะเบียน ให้ยื่นคำขอ พร้อมเอกสารหลักฐานประกอบตามที่กำหนดในคำขอต่อกรมโรงงานอุตสาหกรรม และต้องได้รับความเห็นชอบ เป็นหนังสือจากกรมโรงงานอุตสาหกรรมก่อนจึงจะดำเนินการตามคำขอได้

ข้อ ๑๔ กรณีที่บุคลากรตามหมวด ๒ ลาออก ห้องปฏิบัติการวิเคราะห์เอกซเรย์ต้องแจ้งยกเลิก ทะเบียนบุคลากรต่อกรมโรงงานอุตสาหกรรมภายใน ๓๐ วัน นับแต่วันที่ลาออก

ข้อ ๑๕ การย้ายสถานที่ตั้งของห้องปฏิบัติการวิเคราะห์เอกซเรย์ที่กรมโรงงานอุตสาหกรรม รับขึ้นทะเบียนแล้ว ไปยังสถานที่ตั้งอื่นต้องดำเนินการเสมือนการขอขึ้นทะเบียน เอกซเรย์ใหม่สำหรับสถานที่ใหม่

ข้อ ๑๖ กรณีหนังสือรับขึ้นทะเบียนตามข้อ ๙ หนังสือแสดงการต่ออายุการรับขึ้นทะเบียนตามข้อ ๑๑ หนังสือแสดงการเปลี่ยนแปลงบุคลากรและสารมลพิษห้องปฏิบัติการวิเคราะห์เอกชนตามข้อ ๑๓ สูญหายหรือถูกทำลาย ให้ยื่นคำขอรับหนังสือแทนต่อพนักงานเจ้าหน้าที่ภายใน ๑๕ วัน นับแต่วันที่ทราบถึงการสูญหายหรือถูกทำลาย

ข้อ ๑๗ การเลิกดำเนินการห้องปฏิบัติการวิเคราะห์เอกชนที่กรมโรงงานอุตสาหกรรมรับขึ้นทะเบียนแล้ว ให้แจ้งเป็นหนังสือต่อกรมโรงงานอุตสาหกรรมภายใน ๓๐ วันนับแต่วันเลิกดำเนินการ

ข้อ ๑๘ คำขอขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชนตามข้อ ๘ คำขอต่ออายุการรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชนตามข้อ ๑๑ และคำขอเปลี่ยนแปลงบุคลากรหรือชนิดสารมลพิษวิเคราะห์ ตามข้อ ๑๓ ให้เป็นไปตามแบบที่กรมโรงงานอุตสาหกรรมกำหนด

การยื่นคำขอ การแจ้งตามประกาศนี้ การออกหนังสือรับขึ้นทะเบียนตามข้อ ๙ การออกหนังสือแสดงการต่ออายุการรับขึ้นทะเบียนตามข้อ ๑๑ และการออกหนังสือแสดงการเปลี่ยนแปลงบุคลากรและสารมลพิษตามข้อ ๑๓ ให้ดำเนินการโดยวิธีการทางอิเล็กทรอนิกส์ผ่านระบบเครือข่ายอิเล็กทรอนิกส์ของกรมโรงงานอุตสาหกรรมเป็นหลัก ในกรณีที่ไม่สามารถดำเนินการได้หรือมีเหตุอื่นใดทำให้ไม่สามารถดำเนินการโดยวิธีการทางอิเล็กทรอนิกส์ได้ ให้การดำเนินการดังกล่าวกระทำ ณ กรมโรงงานอุตสาหกรรมหรือหน่วยงานที่กรมโรงงานอุตสาหกรรมกำหนด

หมวด ๕

หน้าที่และความรับผิดชอบ

ข้อ ๑๙ ห้องปฏิบัติการวิเคราะห์เอกชนที่กรมโรงงานอุตสาหกรรมรับขึ้นทะเบียนแล้ว ให้มีหน้าที่และความรับผิดชอบ ดังต่อไปนี้

๑๙.๑ การตรวจวัดสารมลพิษในภาคสนามและหรือเก็บตัวอย่าง น้ำ อากาศ สิ่งปฏิกูลหรือวัสดุที่ไม่ใช้แล้ว ดินและน้ำใต้ดินเพื่อวิเคราะห์ทดสอบภายในห้องปฏิบัติการ ต้องกระทำโดยบุคลากรตามหมวด ๒ เท่านั้น

๑๙.๒ การวิเคราะห์ทดสอบสารมลพิษ น้ำ อากาศ สิ่งปฏิกูลหรือวัสดุที่ไม่ใช้แล้ว ดินและน้ำใต้ดิน ต้องกระทำโดยบุคลากรตามหมวด ๒ เท่านั้น ยกเว้นการวิเคราะห์หาปริมาณ Dioxins/Furans สามารถส่งวิเคราะห์ห้องปฏิบัติการที่ได้รับการขึ้นทะเบียนกับกรมโรงงานอุตสาหกรรม ในรายการ Dioxins/Furans หรือห้องปฏิบัติการของหน่วยงานราชการ หรือห้องปฏิบัติการที่ได้รับการรับรอง ISO/IEC 17025 ได้

๑๙.๓ การรายงานผลการวิเคราะห์ ให้รายงานได้เฉพาะสารมลพิษที่ขึ้นทะเบียนไว้เท่านั้น จากกรมโรงงานอุตสาหกรรมเท่านั้น โดยการรายงานผลการวิเคราะห์ อย่างน้อย ดังนี้

(๑) ชื่อ สถานที่ตั้ง และเลขทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน

- (๒) ชื่อและเลขทะเบียนผู้ควบคุมห้องปฏิบัติการวิเคราะห์เอกชน
- (๓) ผลการตรวจวัด วิเคราะห์ ทดสอบสารมลพิษ
- (๔) ข้อมูลแหล่งที่มาของตัวอย่าง ได้แก่ สถานที่เก็บตัวอย่าง ลักษณะหรือสภาพของตัวอย่าง (ถ้ามี) ชื่อผู้เก็บตัวอย่าง วัน เดือน ปีที่เก็บตัวอย่าง
- (๕) วิธีการตรวจวัดวิเคราะห์ทดสอบ
- (๖) วัน เดือน ปีที่วิเคราะห์ทดสอบ
- (๗) วัน เดือน ปีที่ออกรายงานผล

๑๙.๔ ต้องมีการบันทึกข้อมูลเกี่ยวกับงานที่ปฏิบัติ สภาพตัวอย่างขณะรับเข้าห้องปฏิบัติการ ข้อมูลดิบการตรวจวัด วิเคราะห์ทดสอบ การคำนวณ ผู้วิเคราะห์ และหลักฐานภาพถ่ายการเก็บตัวอย่าง สารมลพิษอากาศ (เว้นแต่มีข้อจำกัดของโรงงานที่ไม่สามารถถ่ายภาพได้) โดยต้องเก็บรักษาข้อมูลและหลักฐานไว้อย่างน้อย ๔ ปีนับแต่เก็บข้อมูลและหลักฐาน

๑๙.๕ ต้องเก็บรักษาสำเนารายงานผลการวิเคราะห์ไว้อย่างน้อย ๔ ปีนับแต่ออกรายงาน

๑๙.๖ ต้องมีการประกันคุณภาพ การควบคุมคุณภาพที่จำเป็นต่อการตรวจวัดวิเคราะห์ทดสอบ และเป็นไปตามวิธีการมาตรฐานที่ใช้อ้างอิง

๑๙.๗ กรณีมีเหตุจำเป็นที่ห้องปฏิบัติการไม่สามารถเก็บตัวอย่าง หรือไม่สามารถวิเคราะห์สารมลพิษ หรือไม่สามารถเก็บตัวอย่างและวิเคราะห์สารมลพิษที่ได้รับขึ้นทะเบียนจากกรมโรงงานอุตสาหกรรมในบางส่วนหรือทั้งหมดได้ จำเป็นต้องมีการจ้างเหมาช่วงห้องปฏิบัติการวิเคราะห์เอกชน ห้องปฏิบัติการวิเคราะห์เอกชนที่เป็นผู้รับจ้างเหมาช่วงต้องได้รับขึ้นทะเบียนรวมทั้งมีขอบข่ายการเก็บตัวอย่างและวิเคราะห์สารมลพิษชนิดที่ได้รับขึ้นทะเบียนจากกรมโรงงานอุตสาหกรรมด้วย กรณีที่รายงานผลการเก็บตัวอย่างหรือการวิเคราะห์ทดสอบได้รวมผลของการวิเคราะห์ที่ดำเนินการโดยผู้รับจ้างเหมาช่วงไว้ด้วย ต้องระบุถึงการจ้างเหมาช่วงและชื่อผู้รับจ้างเหมาช่วงให้ชัดเจนไว้ในรายงานผลการวิเคราะห์ด้วย

๑๙.๘ ห้องปฏิบัติการวิเคราะห์เอกชนต้องยินยอมให้กรมโรงงานอุตสาหกรรมตรวจสอบการดำเนินการของห้องปฏิบัติการวิเคราะห์ที่ได้โดยไม่จำเป็นต้องแจ้งให้ทราบล่วงหน้า

๑๙.๙ ต้องรายงานข้อมูลอื่นตามที่กรมโรงงานอุตสาหกรรมกำหนด

หมวด ๒

มาตรการทางปกครอง

ข้อ ๒๐ ในกรณีที่ปรากฏว่าห้องปฏิบัติการวิเคราะห์เอกชนที่กรมโรงงานอุตสาหกรรมได้รับขึ้นทะเบียนไม่ปฏิบัติตามประกาศนี้ ให้อธิบดีกรมโรงงานอุตสาหกรรมหรือผู้ซึ่งอธิบดีมอบหมายมีอำนาจตักเตือนเป็นหนังสือหรือมีคำสั่งให้แก้ไข หรือปรับ

UNITED ANALYST AND ENGINEERING
CONSULTANT COMPANY LIMITED

ดำเนินการถูกต้อง

ให้ถูกต้องภายในระยะเวลาที่กำหนด และเพื่อประโยชน์ในการควบคุมผลการดำเนินการของห้องปฏิบัติการวิเคราะห์เอกชน กรมโรงงานอุตสาหกรรมอาจแจ้งให้ผู้ให้บริการห้องปฏิบัติการวิเคราะห์เอกชนที่ได้รับผลกระทบทราบ รวมทั้งอาจประกาศรายชื่อห้องปฏิบัติการวิเคราะห์เอกชนดังกล่าวไว้ในที่เปิดเผยก็ได้

ข้อ ๒๑ ในกรณีที่ปรากฏว่าห้องปฏิบัติการวิเคราะห์เอกชนที่กรมโรงงานอุตสาหกรรมได้รับขึ้นทะเบียนแล้ว ผ่าฝืนไม่ปฏิบัติตามคำสั่งตามข้อ ๒๐ หรือเคยฝ่าฝืนไม่ปฏิบัติตามคำสั่งตามข้อ ๒๐ มาแล้วครั้งหนึ่งและมาฝ่าฝืนหรือไม่ปฏิบัติตามคำสั่งตามข้อ ๒๐ อีกภายในระยะเวลา ๑ ปีนับแต่วันฝ่าฝืนไม่ปฏิบัติตามคำสั่งตามข้อ ๒๐ ครั้งก่อน ให้อธิบดีกรมโรงงานอุตสาหกรรมมีอำนาจออกคำสั่งให้พักใช้หนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชนเป็นการชั่วคราวเพื่อให้ดำเนินการแก้ไขหรือปรับปรุงหรือปฏิบัติให้ถูกต้องภายในระยะเวลาที่กำหนด และเพื่อประโยชน์ในการควบคุมผลการดำเนินการของห้องปฏิบัติการวิเคราะห์เอกชน กรมโรงงานอุตสาหกรรมจะประกาศรายชื่อผู้ที่ถูกพักใช้หนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชนไว้ในที่เปิดเผย

ในระหว่างการสั่งพักใช้หนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชนตามวรรคหนึ่ง ให้ถือว่าห้องปฏิบัติการวิเคราะห์เอกชนดังกล่าวไม่ได้รับขึ้นทะเบียนตามประกาศนี้และไม่สามารถขอขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชนใหม่ได้จนกว่าจะสิ้นสุดระยะเวลาการพักใช้หนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน

ข้อ ๒๒ ในกรณีที่ปรากฏว่า ห้องปฏิบัติการวิเคราะห์เอกชนที่กรมโรงงานอุตสาหกรรมได้รับขึ้นทะเบียนแล้ว ผ่าฝืนหรือไม่ดำเนินการแก้ไขหรือปรับปรุงหรือปฏิบัติให้ถูกต้องตามที่ได้มีคำสั่งพักใช้หนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน ตามข้อ ๒๑ โดยไม่มีเหตุอันสมควรหรือมีเจตนารายงานผลอันเป็นเท็จ ให้อธิบดีกรมโรงงานอุตสาหกรรมมีอำนาจเพิกถอนการรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชนและให้ถือว่าการเพิกถอนการรับขึ้นทะเบียนตามข้อนี้เป็นการยกเลิกหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชนตั้งแต่วันที่เพิกถอนการรับขึ้นทะเบียน และเพื่อประโยชน์ในการควบคุมผลการดำเนินการของห้องปฏิบัติการวิเคราะห์เอกชน กรมโรงงานอุตสาหกรรมจะประกาศรายชื่อผู้ถูกเพิกถอนการรับขึ้นทะเบียนดังกล่าวไว้ในที่เปิดเผย นอกจากนี้กรมโรงงานอุตสาหกรรมจะไม่รับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชนรายนี้อีกจนกว่าจะพ้นกำหนด ๔ ปีนับแต่วันที่เพิกถอนการรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน

ผลแห่งการเพิกถอนการรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชนให้ถือว่าห้องปฏิบัติการวิเคราะห์เอกชนดังกล่าวมิได้รับการขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชนตามประกาศนี้

หมวด ๗

บทเฉพาะกาล

ข้อ ๒๓ หนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชนที่กรมโรงงานอุตสาหกรรมออกก่อนวันที่ประกาศนี้มีผลใช้บังคับ ให้ใช้บังคับต่อไปจนกว่าจะสิ้นอายุ ในการออกใบรับขึ้นทะเบียนดังกล่าวให้ถือว่าเป็น

CONSULTANT COMPANY LIMITED

การต่ออายุการรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชนตามข้อ ๑๑ ให้ดำเนินการตามประกาศนี้ โดยอนุโลม ทั้งนี้ ห้องปฏิบัติการวิเคราะห์เอกชนดังกล่าวต้องปฏิบัติตามประกาศนี้ต่อไปด้วย

ภายในระยะเวลา ๑ ปี นับแต่วันที่ประกาศนี้มีผลใช้บังคับ การดำเนินการต่ออายุหนังสือการรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชนตามวรรคหนึ่งให้ได้รับยกเว้นการส่งเอกสารข้อมูลการตรวจวัดและเก็บตัวอย่างสารมลพิษอากาศตามข้อ ๑๑ วรรคสาม

ข้อ ๒๔ คำขอใด ๆ ที่เกี่ยวข้องกับการขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชนที่ได้ยื่นไว้ ก่อนวันที่ประกาศนี้ใช้บังคับแต่ยังพิจารณาไม่แล้วเสร็จในวันที่ประกาศนี้ใช้บังคับ ให้নাประกาศนี้มาใช้บังคับกับการพิจารณาคำขอโดยอนุโลมเท่าที่จะทำได้ และเพื่อประโยชน์ของการดำเนินการตามข้อนี้ ให้เจ้าหน้าที่ มีอำนาจเรียกเอกสารหรือข้อเท็จจริงใด ๆ จากผู้ยื่นคำขอหรือให้ผู้ยื่นคำขอมาชี้แจงใด ๆ เพื่อประกอบการพิจารณาก็ได้

ประกาศ ณ วันที่ ๑๕ ธันวาคม พ.ศ. ๒๕๖๖

อธิบดีกรมโรงงานอุตสาหกรรม

UAE

UNITED ANALYST AND ENGINEERING
CONSULTANT COMPANY LIMITED

สำนักงานกรุงเทพมหานคร

ภาคผนวก ก

วุฒิการศึกษาของผู้ควบคุมห้องปฏิบัติการวิเคราะห์เอกซเรณและเจ้าหน้าที่ห้องปฏิบัติการวิเคราะห์เอกซเรณ
ที่สามารถขึ้นทะเบียนกับกรมโรงงานอุตสาหกรรม

๑. วิทยาศาสตร์บัณฑิต วิทยาศาสตร์มหาบัณฑิต วิทยาศาสตรดุษฎีบัณฑิต หรือปรัชญาดุษฎีบัณฑิต
สาขาดังต่อไปนี้

- | | |
|--|---|
| ๑.๑ เคมี | ๑.๑๕ ชีวเคมี |
| ๑.๒ เคมีเทคนิค | ๑.๑๖ ธรณีวิทยา |
| ๑.๓ เคมี-ชีววิทยา | ๑.๑๗ วิทยาการสิ่งแวดล้อมและทรัพยากรธรรมชาติ |
| ๑.๔ เคมีทรัพยากรธรรมชาติ | ๑.๑๘ วิทยาศาสตร์และเทคโนโลยีสิ่งแวดล้อม |
| ๑.๕ เคมีวิเคราะห์ | ๑.๑๙ วิทยาศาสตร์ชีวภาพ |
| ๑.๖ เคมีสิ่งแวดล้อม | ๑.๒๐ วิทยาศาสตร์ทั่วไป |
| ๑.๗ เคมีอินทรีย์ | ๑.๒๑ วิทยาศาสตร์สิ่งแวดล้อม |
| ๑.๘ เคมีอุตสาหกรรม | ๑.๒๒ วิทยาศาสตร์สุขภาพ |
| ๑.๙ เทคโนโลยีและการจัดการสิ่งแวดล้อม | ๑.๒๓ สาธารณสุขศาสตร์ |
| ๑.๑๐ เทคโนโลยีชีวภาพ | ๑.๒๔ สิ่งแวดล้อม |
| ๑.๑๑ เทคโนโลยีสิ่งแวดล้อม | ๑.๒๕ สุขศาสตร์อุตสาหกรรมและความปลอดภัย |
| ๑.๑๒ การจัดการทรัพยากรดินและสิ่งแวดล้อม | ๑.๒๖ สุขาภิบาล |
| ๑.๑๓ การจัดการสิ่งแวดล้อมเมือง และอุตสาหกรรม | ๑.๒๗ อนามัยสิ่งแวดล้อม |
| ๑.๑๔ จุลชีววิทยา | ๑.๒๘ อชีวอนามัยและความปลอดภัย |

๒. วิศวกรรมศาสตรบัณฑิต สาขาวิศวกรรมเคมี สาขาวิศวกรรมปิโตรเคมี หรือสาขาวิศวกรรมสิ่งแวดล้อม

๓. การศึกษามัธยมศึกษา/ครุศาสตรบัณฑิต/ศึกษาศาสตรบัณฑิต สาขาเคมี หรือสาขาวิทยาศาสตร์ทั่วไป

ภาคผนวก ข

หน่วยงานและรูปแบบการฝึกอบรมที่กรมโรงงานอุตสาหกรรมเห็นชอบ

เพื่อให้บุคลากรของห้องปฏิบัติการได้มีความรู้ ความเข้าใจ เกี่ยวกับข้อกำหนดทั่วไปว่าด้วยความสามารถของห้องปฏิบัติการทดสอบและ/หรือสอบเทียบ มอก. ๑๙๐๒๕ (ISO/IEC 17025) และ การควบคุมคุณภาพการวิเคราะห์ นำมาซึ่งการใช้ในงานวิเคราะห์ที่ปฏิบัติประจำในห้องปฏิบัติการวิเคราะห์เอกชนที่ขึ้นทะเบียนกับกรมโรงงานอุตสาหกรรม

ให้หน่วยงานดังต่อไปนี้เป็นหน่วยงานฝึกอบรมโดยให้มีรูปแบบการจัดฝึกอบรมเป็นแบบฝึกอบรมนอกสถานที่ (public training) ฝึกอบรมภายในองค์กร (in-house training) หรือฝึกอบรมสดผ่านระบบออนไลน์ (virtual training)

๑. กรมโรงงานอุตสาหกรรม
๒. หน่วยงานราชการ หรือหน่วยงานในกำกับของรัฐ หรือรัฐวิสาหกิจ ได้แก่
 - ๒.๑ กรมวิทยาศาสตร์บริการ
 - ๒.๒ สำนักงานมาตรฐานผลิตภัณฑ์อุตสาหกรรม
 - ๒.๓ สถาบันมาตรวิทยาแห่งชาติ
 - ๒.๔ สถาบันวิจัยวิทยาศาสตร์และเทคโนโลยีแห่งประเทศไทย
 - ๒.๕ สถาบันอาหาร
 - ๒.๖ สถาบันรับรองมาตรฐานไอเอสโอ
๓. หน่วยงานอื่นที่กรมโรงงานอุตสาหกรรมเห็นชอบเพิ่มเติม



๐ ๓ พฤษภาคม ๒๕๖๗

เรื่อง เปลี่ยนแปลงบุคลากร สारมลพิษที่วิเคราะห์และเอกสารอ้างอิงวิธีวิเคราะห์สารมลพิษ

เรียน กรรมการผู้จัดการ บริษัท ยูโนเด็ด แอนนาลิสต์ แอนด์ เอ็นจิเนียริง คอนซัลแตนท์ จำกัด

อ้างถึง ๑. คำขอขึ้นทะเบียน/ต่ออายุ/เปลี่ยนแปลงบุคลากร และชนิดสารมลพิษของห้องปฏิบัติการวิเคราะห์เอกชน

ลงวันที่ ๔ มีนาคม ๒๕๖๗

๒. คำขอขึ้นทะเบียน/ต่ออายุ/เปลี่ยนแปลงบุคลากร และชนิดสารมลพิษของห้องปฏิบัติการวิเคราะห์เอกชน

ลงวันที่ ๑๒ มีนาคม ๒๕๖๗

สิ่งที่ส่งมาด้วย เอกสารแนบท้ายหนังสือเปลี่ยนแปลงบุคลากร สารมลพิษที่วิเคราะห์และเอกสารอ้างอิง

วิธีวิเคราะห์สารมลพิษ บริษัท ยูโนเด็ด แอนนาลิสต์ แอนด์ เอ็นจิเนียริง คอนซัลแตนท์ จำกัด

จำนวน ๑๙ แผ่น


ตามคำขอที่อ้างถึง ๑ และ ๒ บริษัท ยูโนเด็ด แอนนาลิสต์ แอนด์ เอ็นจิเนียริง คอนซัลแตนท์ จำกัด


ห้องปฏิบัติการวิเคราะห์เอกชน เลขทะเบียน ๖-๑๔๕ สถานที่ตั้งเลขที่ ๓ ซอยอุดมสุข ๔๑ ถนนสุขุมวิท แขวงบางจาก

เขตพระโขนง กรุงเทพมหานคร ขอเปลี่ยนแปลงบุคลากร สารมลพิษที่วิเคราะห์และเอกสารอ้างอิงวิธีวิเคราะห์

สารมลพิษ ความละเอียดแจ้งแล้ว นั้น

กรมโรงงานอุตสาหกรรมพิจารณาแล้ว มีความเห็นให้เปลี่ยนแปลงดังนี้






๔. ให้ยกเลิกขบข่ายรายการสารมลพิษในน้ำเสีย น้ำใต้ดิน และสิ่งปฏิกูลหรือวัสดุที่ไม่ใช้แล้ว ตามรายการเอกสารแนบท้ายหนังสือต่ออายุรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน ที่ อก ๐๓๑๐(๑)/๑๘๗๙ ลงวันที่ ๙ กุมภาพันธ์ ๒๕๖๕

๕. ให้วิเคราะห์สารมลพิษตามขบข่ายที่ได้รับขึ้นทะเบียนให้วิเคราะห์ในน้ำ/น้ำเสีย น้ำใต้ดิน และสิ่งปฏิกูลหรือวัสดุที่ไม่ใช้แล้ว ตามเอกสารแนบท้ายหนังสือเปลี่ยนแปลงบุคลากร สารมลพิษที่วิเคราะห์และเอกสารอ้างอิงวิธีวิเคราะห์สารมลพิษ ดังสิ่งที่ส่งมาด้วย

อนึ่ง หนังสือฉบับนี้จะหมดอายุพร้อมหนังสือต่ออายุรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน ในวันที่ ๒ กุมภาพันธ์ ๒๕๖๘

จึงเรียนมาเพื่อทราบ

ขอแสดงความนับถือ



รองอธิบดี ปฏิบัติราชการแทน
อธิบดีกรมโรงงานอุตสาหกรรม

กองวิจัยและเตือนภัยมลพิษโรงงาน

กลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษและทะเบียนห้องปฏิบัติการ

โทร. ๐ ๒๔๓๐ ๖๓๑๒ ต่อ ๒๑๐๓-๕

โทรสาร ๐ ๒๔๓๐ ๖๓๑๒ ต่อ ๒๑๑๙

โปรเจกต์อิเล็กทรอนิกส์ saraban@diw.mail.go.th



“อุตสาหกรรมก้าวไกล ประเทศไทยก้าวหน้า ร่วมกันพัฒนา อุตสาหกรรมสีเขียว”



ด้าน เกษตร



เอกสารแนบท้ายหนังสือเปลี่ยนแปลงบุคลากร สารมลพิษที่วิเคราะห์และเอกสารอ้างอิงวิธีวิเคราะห์สารมลพิษ
บริษัท ยูไนเต็ด แอนนาลิสต์ แอนด์ เอ็นจิเนียริง คอนซัลแตนท์ จำกัด เลขทะเบียน ๖-๑๔๕
ที่ อก ๐๓๑๐(๑)/ ๔๓๓๕ I ลงวันที่ ๐๓ พฤษภาคม ๒๕๖๗

ขอบข่ายสารมลพิษที่ได้รับขึ้นทะเบียนจากกรมโรงงานอุตสาหกรรม จำนวน ๒๐๗ รายการ

น้ำ/น้ำเสีย จำนวน 46 รายการ

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
1	Aldrin	Liquid-Liquid Extraction, Gas Chromatographic Method ^[3]
2	Arsenic	1) Digestion, Hydride Generation/Atomic Absorption Spectrometric Method ^[3] 2) Digestion, Inductively Coupled Plasma Method ^[3]
3	Barium	Digestion, Inductively Coupled Plasma Method ^[3]
4	α-BHC	Liquid-Liquid Extraction, Gas Chromatographic Method ^[3]
5	β-BHC	Liquid-Liquid Extraction, Gas Chromatographic Method ^[3]
6	δ-BHC	Liquid-Liquid Extraction, Gas Chromatographic Method ^[3]
7	γ-BHC	Liquid-Liquid Extraction, Gas Chromatographic Method ^[3]
8	Biochemical Oxygen Demand	1) 5-Day BOD Test, Azide Modification Method ^[3] 2) 5-Day BOD Test, Membrane Electrode Method ^[3]
9	Cadmium	1) Digestion, Direct Air-Acetylene Flame Method ^[3] 2) Digestion, Electrothermal Atomic Absorption Spectrometric Method ^[3] 3) Digestion, Inductively Coupled Plasma Method ^[3]
10	Chemical Oxygen Demand	1) Closed Reflux, Titrimetric Method ^[3] 2) Closed Reflux, Colorimetric Method ^[3] 3) Open Reflux, Titrimetric Method ^[3]
11	Chlordane	Liquid-Liquid Extraction, Gas Chromatographic Method ^[3]
12	Chromium	1) Digestion, Direct Air-Acetylene Flame Method ^[3] 2) Digestion, Electrothermal Atomic Absorption Spectrometric Method ^[3] 3) Digestion, Inductively Coupled Plasma Method ^[3]
13	Color	ADMI Weighted-Ordinate Spectrophotometric Method ^[3]
14	Copper	1) Digestion, Direct Air-Acetylene Flame Method ^[3] 2) Digestion, Electrothermal Atomic Absorption Spectrometric Method ^[3] 3) Digestion, Inductively Coupled Plasma Method ^[3]
15	Cyanide	1) Distillation, Colorimetric Method ^[3] 2) Flow Injection Analysis Method ^[3]
16	o,p'-DDT	Liquid-Liquid Extraction, Gas Chromatographic Method ^[3]

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
17	4,4'-DDD	Liquid-Liquid Extraction, Gas Chromatographic Method ^[3]
18	4,4'-DDE	Liquid-Liquid Extraction, Gas Chromatographic Method ^[3]
19	4,4'-DDT	Liquid-Liquid Extraction, Gas Chromatographic Method ^[3]
20	Dieldrin	Liquid-Liquid Extraction, Gas Chromatographic Method ^[3]
21	Endosulfan I	Liquid-Liquid Extraction, Gas Chromatographic Method ^[3]
22	Endosulfan II	Liquid-Liquid Extraction, Gas Chromatographic Method ^[3]
23	Endosulfan sulfate	Liquid-Liquid Extraction, Gas Chromatographic Method ^[3]
24	Endrin	Liquid-Liquid Extraction, Gas Chromatographic Method ^[3]
25	Endrin aldehyde	Liquid-Liquid Extraction, Gas Chromatographic Method ^[3]
26	Formaldehyde	Distillation, Colorimetric Method ^[2]
27	Free Chlorine	1) Iodometric Method ^[3] 2) DPD Ferrous Titrimetric Method ^[3]
28	Heptachlor	Liquid-Liquid Extraction, Gas Chromatographic Method ^[3]
29	Heptachlor Epoxide	Liquid-Liquid Extraction, Gas Chromatographic Method ^[3]
30	Hexavalent Chromium	1) Colorimetric Method ^[3] 2) Extraction, Direct Air Acetylene Flame Method ^[3]
31	Lead	1) Digestion, Direct Air-Acetylene Flame Method ^[3] 2) Digestion, Electrothermal Atomic Absorption Spectrometric Method ^[3] 3) Digestion, Inductively Coupled Plasma Method ^[3]
32	Manganese	1) Digestion, Direct Air-Acetylene Flame Method ^[3] 2) Digestion, Electrothermal Atomic Absorption Spectrometric Method ^[3] 3) Digestion, Inductively Coupled Plasma Method ^[3]
33	Mercury	Digestion, Cold-Vapor Atomic Absorption Spectrometric Method ^[3]
34	Methoxychlor	Liquid-Liquid Extraction, Gas Chromatographic Method ^[3]
35	Nickel	1) Digestion, Direct Air-Acetylene Flame Method ^[3] 2) Digestion, Electrothermal Atomic Absorption Spectrometric Method ^[3] 3) Digestion, Inductively Coupled Plasma Method ^[3]
36	Oil & Grease	1) Liquid-Liquid, Partition Gravimetric Method ^[3] 2) Soxhlet Extraction Method ^[3]
37	pH	Electrometric Method ^[3]

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
38	Phenols	1) Distillation, Chloroform Extraction Method ^[3] 2) Distillation, Direct Photometric Method ^[3]
39	Selenium	1) Digestion, Hydride Generation/Atomic Absorption Spectrometric Method ^[3] 2) Digestion, Inductively Coupled Plasma Method ^[3]
40	Sulfide	1) Iodometric Method ^[3] 2) Methylene Blue Method ^[3]
41	Temperature	Laboratory and Field Methods ^[3]
42	Total Dissolved Solids	Dried at 180 °C ^[3]
43	Total Kjeldahl Nitrogen	Semi-Micro-Kjeldahl Method ^[3]
44	Total Suspended Solids	Dried from 103 to 105 °C ^[3]
45	Trivalent Chromium	1) Digestion, Direct Air-Acetylene Flame Method; Colorimetric Method; Calculation ^[3] 2) Digestion, Inductively Coupled Plasma Method; Colorimetric Method; Calculation ^[3]
46	Zinc	1) Digestion, Direct Air-Acetylene Flame Method ^[3] 2) Digestion, Electrothermal Atomic Absorption Spectrometric Method ^[3] 3) Digestion, Inductively Coupled Plasma Method ^[3]

น้ำใต้ดิน จำนวน 126 รายการ

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
1	Acenaphthene	1) Liquid-Liquid Extraction, Gas Chromatographic Method ^[3] 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[3]
2	Acetone	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ^[3]
3	Aldrin	1) Liquid-Liquid Extraction, Gas Chromatographic Method ^[3] 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[3]
4	Anthracene	1) Liquid-Liquid Extraction, Gas Chromatographic Method ^[3] 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[3]

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
5	Antimony	Digestion, Inductively Coupled Plasma Method ^[3]
6	Arsenic	1) Digestion, Hydride Generation/Atomic Absorption Spectrometric Method ^[3] 2) Digestion, Inductively Coupled Plasma Method ^[3]
7	Atrazine	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[3]
8	Barium	1) Digestion, Electrothermal Atomic Absorption Spectrometric Method ^[3] 2) Digestion, Inductively Coupled Plasma Method ^[3]
9	Benz(a)anthracene	1) Liquid-Liquid Extraction, Gas Chromatographic Method ^[3] 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[3]
10	Benzene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ^[3]
11	Benzo(b)fluoranthene	1) Liquid-Liquid Extraction, Gas Chromatographic Method ^[3] 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[3]
12	Benzo(k)fluoranthene	1) Liquid-Liquid Extraction, Gas Chromatographic Method ^[3] 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[3]
13	Benzoic acid	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[3]
14	Benzo(a)pyrene	1) Liquid-Liquid Extraction, Gas Chromatographic Method ^[3] 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[3]
15	Benzo(g,h,i)perylene	1) Liquid-Liquid Extraction, Gas Chromatographic Method ^[3] 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[3]
16	Beryllium	Digestion, Inductively Coupled Plasma Method ^[3]
17	Bis(2-chloroethyl)ether	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[3]
18	Bis(2-ethylhexyl)phthalate	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[3]

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
19	Bromodichloromethane	Purge and Trap Gas Chromatographic/ Mass Spectrometric Method ^[3]
20	Bromoform	Purge and Trap Gas Chromatographic/ Mass Spectrometric Method ^[3]
21	Butanol	Purge and Trap Gas Chromatographic/ Mass Spectrometric Method ^[3]
22	Butyl benzyl phthalate	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[3]
23	Cadmium	1) Digestion, Direct Air-Acetylene Flame Method ^[3] 2) Digestion, Electrothermal Atomic Absorption Spectrometric Method ^[3] 3) Digestion, Inductively Coupled Plasma Method ^[3]
24	Carbazole	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[3]
25	Carbon disulfide	Purge and Trap Gas Chromatographic/ Mass Spectrometric Method ^[3]
26	Carbon tetrachloride	Purge and Trap Gas Chromatographic/ Mass Spectrometric Method ^[3]
27	Chlordane	1) Liquid-Liquid Extraction, Gas Chromatographic Method ^[3] 2) Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[3]
28	p-Chloroaniline	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[3]
29	Chlorobenzene	Purge and Trap Gas Chromatographic/ Mass Spectrometric Method ^[3]
30	Chlorodibromomethane	Purge and Trap Gas Chromatographic/ Mass Spectrometric Method ^[3]
31	Chloroform	Purge and Trap Gas Chromatographic/ Mass Spectrometric Method ^[3]
32	2-Chlorophenol	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[3]
33	Chromium	1) Digestion, Direct Air-Acetylene Flame Method ^[3] 2) Digestion, Electrothermal Atomic Absorption Spectrometric Method ^[3] 3) Digestion, Inductively Coupled Plasma Method ^[3]

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
34	Chromium (III)	1) Digestion, Direct Air-Acetylene Flame Method; Colorimetric Method; Calculation ^[3] 2) Digestion, Inductively Coupled Plasma Method; Colorimetric Method; Calculation ^[3]
35	Chromium (VI)	1) Colorimetric Method ^[3] 2) Extraction, Air-Acetylene Flame Method ^[3]
36	Chrysene	1) Liquid-Liquid Extraction, Gas Chromatographic Method ^[3] 2) Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[3]
37	Cyanide	Distillation, Colorimetric Method ^[3]
38	2,4-D	Liquid-Liquid Extraction, Gas Chromatographic Method ^[3]
39	DDO	1) Liquid-Liquid Extraction, Gas Chromatographic Method ^[3] 2) Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[3]
40	DDE	1) Liquid-Liquid Extraction, Gas Chromatographic Method ^[3] 2) Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[3]
41	DDT	1) Liquid-Liquid Extraction, Gas Chromatographic Method ^[3] 2) Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[3]
42	Dibenz(a,h)anthracene	1) Liquid-Liquid Extraction, Gas Chromatographic Method ^[3] 2) Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[3]
43	Di-n-butyl phthalate	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[3]
44	1,2-Dichlorobenzene	Purge and Trap Gas Chromatographic/ Mass Spectrometric Method ^[3]
45	1,3-Dichlorobenzene	Purge and Trap Gas Chromatographic/ Mass Spectrometric Method ^[3]
46	1,4-Dichlorobenzene	Purge and Trap Gas Chromatographic/ Mass Spectrometric Method ^[3]
47	3,3'-Dichlorobenzidine	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[3]

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
48	1,1-Dichloroethane	Purge and Trap Gas Chromatographic/ Mass Spectrometric Method ^[3]
49	1,2-Dichloroethane	Purge and Trap Gas Chromatographic/ Mass Spectrometric Method ^[3]
50	1,1-Dichloroethylene	Purge and Trap Gas Chromatographic/ Mass Spectrometric Method ^[3]
51	cis-1,2-Dichloroethylene	Purge and Trap Gas Chromatographic/ Mass Spectrometric Method ^[3]
52	trans-1,2-Dichloroethylene	Purge and Trap Gas Chromatographic/ Mass Spectrometric Method ^[3]
53	2,4-Dichlorophenol	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[3]
54	1,2 Dichloropropane	Purge and Trap Gas Chromatographic/ Mass Spectrometric Method ^[3]
55	1,3-Dichloropropane	Purge and Trap Gas Chromatographic/ Mass Spectrometric Method ^[3]
56	1,3-Dichloropropene	Purge and Trap Gas Chromatographic/ Mass Spectrometric Method ^[3]
57	Dieldrin	1) Liquid-Liquid Extraction, Gas Chromatographic Method ^[3] 2) Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[3]
58	Diethyl phthalate	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[3]
59	2,4-Dimethylphenol	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[3]
60	2,4-Dinitrophenol	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[3]
61	2,4-Dinitrotoluene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[3]
62	2,6-Dinitrotoluene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[3]
63	Di-n-Octyl phthalate	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[3]
64	Endosulfan	1) Liquid-Liquid Extraction, Gas Chromatographic Method ^[3] 2) Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[3]

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
65	Endrin	1) Liquid-Liquid Extraction, Gas Chromatographic Method ^[3] 2) Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[3]
66	Ethylbenzene	Purge and Trap Gas Chromatographic/ Mass Spectrometric Method ^[3]
67	Fluoranthene	1) Liquid-Liquid Extraction, Gas Chromatographic Method ^[3] 2) Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[3]
68	Fluorene	1) Liquid-Liquid Extraction, Gas Chromatographic Method ^[3] 2) Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[3]
69	Heptachlor	1) Liquid-Liquid Extraction, Gas Chromatographic Method ^[3] 2) Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[3]
70	Heptachlor epoxide	1) Liquid-Liquid Extraction, Gas Chromatographic Method ^[3] 2) Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[3]
71	Hexachlorobenzene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[3]
72	Hexachloro-1,3-butadiene	Purge and Trap Gas Chromatographic/ Mass Spectrometric Method ^[3]
73	n-Hexane	Purge and Trap Gas Chromatographic/ Mass Spectrometric Method ^[3]
74	α -HCH	1) Liquid-Liquid Extraction, Gas Chromatographic Method ^[3] 2) Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[3]
75	β -HCH	1) Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[3] 2) Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[3]

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
76	γ -HCH	1) Liquid-Liquid Extraction, Gas Chromatographic Method ^[3] 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[3]
77	Hexachlorocyclopentadiene	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[3]
78	Hexachloroethane	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[3]
79	Indeno(1,2,3-cd)pyrene	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[3]
80	Isophorone	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[3]
81	Lead	1) Digestion, Direct Air-Acetylene Flame Method ^[3] 2) Digestion, Electrothermal Atomic Absorption Spectrometric Method ^[3] 3) Digestion, Inductively Coupled Plasma Method ^[3]
82	Manganese	1) Digestion, Direct Air-Acetylene Flame Method ^[3] 2) Digestion, Electrothermal Atomic Absorption Spectrometric Method ^[3] 3) Digestion, Inductively Coupled Plasma Method ^[3]
83	Mercury	Digestion, Cold-Vapor Atomic Absorption Spectrometric Method ^[3]
84	Methanol	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ^[3]
85	Methoxychlor	Liquid-Liquid Extraction, Gas Chromatographic Method ^[3]
86	Methyl bromide	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ^[3]
87	Methylene chloride	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ^[3]
88	2-Methylphenol	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[3]
89	2-Methylnaphthalene	1) Liquid-Liquid Extraction, Gas Chromatographic Method ^[3] 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[3]
90	Methyl tert-butyl ether	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ^[3]

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
91	Naphthalene	1) Liquid-Liquid Extraction, Gas Chromatographic Method ^[3] 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[3]
92	Nickel	1) Digestion, Direct Air-Acetylene Flame Method ^[3] 2) Digestion, Electrothermal Atomic Absorption Spectrometric Method ^[3] 3) Digestion, Inductively Coupled Plasma Method ^[3]
93	Nitrobenzene	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[3]
94	N-Nitrosodiphenylamine	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[3]
95	N-Nitrosodi-n-propylamine	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[3]
96	Polychlorinated Biphenyls - PCB 1016 - PCB 1221 - PCB 1232 - PCB-1242 - PCB-1248 - PCB-1254 - PCB-1260	1) Liquid-Liquid Extraction, Gas Chromatographic Method ^[3] 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[3]
97	Pentachlorophenol	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[3]
98	pH	Electrometric Method ^[3]
99	Phenanthrene	1) Liquid-Liquid Extraction, Gas Chromatographic Method ^[3] 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[3]
100	Phenol	1) Distillation, Chloroform Extraction Method ^[3] 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[3]
101	Pyrene	1) Liquid-Liquid Extraction, Gas Chromatographic Method ^[3] 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[3]

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
102	Selenium	1) Digestion, Hydride Generation/Atomic Absorption Spectrometric Method ^[3] 2) Digestion, Inductively Coupled Plasma Method ^[3]
103	Silver	Digestion, Inductively Coupled Plasma Method ^[3]
104	Styrene	Purge and Trap Gas Chromatographic/ Mass Spectrometric Method ^[3]
105	1,1,2,2-Tetrachloroethane	Purge and Trap Gas Chromatographic/ Mass Spectrometric Method ^[3]
106	Tetrachloroethylene	Purge and Trap Gas Chromatographic/ Mass Spectrometric Method ^[3]
107	Toluene	Purge and Trap Gas Chromatographic/ Mass Spectrometric Method ^[3]
108	Toxaphene	1) Liquid-Liquid Extraction, Gas Chromatographic Method ^[3] 2) Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[3]
109	TPH (C ₅ - C ₈)	1) Purge and Trap, Gas Chromatographic Method ^[10,20] 2) Purge and Trap, Gas Chromatographic/ Mass spectrometric Method ^[10,23]
110	TPH (C ₉ - C ₁₆)	Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method ^[7,20]
111	TPH (C ₁₇ - C ₃₅)	Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method ^[7,20]
112	1,2,4-Trichlorobenzene	Purge and Trap Gas Chromatographic/ Mass Spectrometric Method ^[3]
113	1,1,1-Trichloroethane	Purge and Trap Gas Chromatographic/ Mass Spectrometric Method ^[3]
114	1,1,2-Trichloroethane	Purge and Trap Gas Chromatographic/ Mass Spectrometric Method ^[3]
115	Trichloroethylene	Purge and Trap Gas Chromatographic/ Mass Spectrometric Method ^[3]
116	2,4,5-Trichlorophenol	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[3]
117	2,4,6-Trichlorophenol	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[3]
118	1,3,5-Trimethylbenzene	Purge and Trap Gas Chromatographic/ Mass Spectrometric Method ^[3]

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
119	Vanadium	Digestion, Inductively Coupled Plasma Method ^[3]
120	Vinyl acetate	Purge and Trap Gas Chromatographic/ Mass Spectrometric Method ^[3]
121	Vinyl chloride	Purge and Trap Gas Chromatographic/ Mass Spectrometric Method ^[3]
122	m-Xylene	Purge and Trap Gas Chromatographic/ Mass Spectrometric Method ^[3]
123	o-Xylene	Purge and Trap Gas Chromatographic/ Mass Spectrometric Method ^[3]
124	p-Xylene	Purge and Trap Gas Chromatographic/ Mass Spectrometric Method ^[3]
125	Xylene (Total)	Purge and Trap Gas Chromatographic/ Mass Spectrometric Method ^[3]
126	Zinc	1) Digestion, Direct Air-Acetylene Flame Method ^[3] 2) Digestion, Electrothermal Atomic Absorption Spectrometric Method ^[3] 3) Digestion, Inductively Coupled Plasma Method ^[3]

สิ่งปฏิกูลหรือวัสดุที่ไม่ใช้แล้ว จำนวน 35 รายการ

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
1	Aldrin	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method ^[1,7,21] 2) Ultrasonic Extraction, Gas Chromatographic Method ^[8,21]
2	Antimony	Digestion, Inductively Coupled Plasma Method ^[5,12]
3	Arsenic	1) Waste Extraction, Digestion, Hydride Generation/Atomic Absorption Spectrometric Method ^[1,4,14] 2) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[1,4,12] 3) Digestion, Hydride Generation/Atomic Absorption Spectrometric Method ^[9,14] 4) Digestion, Inductively Coupled Plasma Method ^[5,12]
4	Barium	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[1,4,12] 2) Digestion, Inductively Coupled Plasma Method ^[5,12]

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
5	Beryllium	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[1,4,12]
6	Cadmium	2) Digestion, Inductively Coupled Plasma Method ^[5,12] 1) Waste Extraction, Digestion, Flame Atomic Absorption Spectrometric Method ^[1,4,13] 2) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[1,4,12] 3) Digestion, Flame Atomic Absorption Spectrometric Method ^[5,13] 4) Digestion, Inductively Coupled Plasma Method ^[5,12]
7	Chlordane	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method ^[1,7,21] 2) Ultrasonic Extraction, Gas Chromatographic Method ^[8,21]
8	Chromium	1) Waste Extraction, Digestion, Flame Atomic Absorption Spectrometric Method ^[1,4,13] 2) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[1,4,12] 3) Digestion, Flame Atomic Absorption Spectrometric Method ^[5,13] 4) Digestion, Inductively Coupled Plasma Method ^[5,12]
9	Chromium (III)	1) Waste Extraction, Digestion, Flame Atomic Absorption Spectrometric Method; Waste Extraction, Colorimetric Method; Calculation ^[1,4,13,15] 2) Waste Extraction, Digestion, Inductively Coupled Plasma Method; Waste Extraction, Colorimetric Method; Calculation ^[1,4,12,15] 3) Digestion, Flame Atomic Absorption Spectrometric Method; Alkaline Digestion, Colorimetric Method; Calculation ^[5,6,13,15] 4) Digestion, Inductively Coupled Plasma Method; Alkaline Digestion, Colorimetric Method; Calculation ^[5,6,12,15]
10	Chromium (VI)	1) Waste Extraction, Colorimetric Method 2) Alkaline Digestion, Colorimetric Method ^[6,15]
11	Cobalt	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[1,4,12] 2) Digestion, Inductively Coupled Plasma Method ^[5,12]

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
12	Copper	1) Waste Extraction, Digestion, Flame Atomic Absorption Spectrometric Method ^[1,4,13] 2) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[1,4,12] 3) Digestion, Flame Atomic Absorption Spectrometric Method ^[5,13] 4) Digestion, Inductively Coupled Plasma Method ^[5,12]
13	2,4-D	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method ^[1,7,21] 2) Ultrasonic Extraction, Gas Chromatographic Method ^[8,21]
14	DDD	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method ^[1,7,21] 2) Ultrasonic Extraction, Gas Chromatographic Method ^[8,21]
15	DDE	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method ^[1,7,21] 2) Ultrasonic Extraction, Gas Chromatographic Method ^[8,21]
16	DDT	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method ^[1,7,21] 2) Ultrasonic Extraction, Gas Chromatographic Method ^[8,21]
17	Dieldrin	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method ^[1,7,21] 2) Ultrasonic Extraction, Gas Chromatographic Method ^[8,21]
18	Endrin	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method ^[1,7,21] 2) Ultrasonic Extraction, Gas Chromatographic Method ^[8,21]
19	Heptachlor	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method ^[1,7,21] 2) Ultrasonic Extraction, Gas Chromatographic Method ^[8,21]

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
20	Lead	1) Waste Extraction, Digestion, Flame Atomic Absorption Spectrometric Method ^[1,4,13] 2) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[1,4,12] 3) Digestion, Flame Atomic Absorption Spectrometric Method ^[5,13] 4) Digestion, Inductively Coupled Plasma Method ^[5,12]
21	Lindane	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method ^[1,7,21] 2) Ultrasonic Extraction, Gas Chromatographic Method ^[8,21]
22	Mercury	1) Waste Extraction, Digestion, Cold-Vapor Atomic Absorption Spectrometric Method ^[1,16] 2) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[1,4,12] 3) Digestion, Cold-Vapor Atomic Absorption Spectrometric Method ^[17] 4) Digestion, Inductively Coupled Plasma Method ^[5,12] 5) Thermal Decomposition Amalgamation and Atomic Absorption Spectrometric Method ^[18]
23	Methoxychlor	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method ^[1,7,21] 2) Ultrasonic Extraction, Gas Chromatographic Method ^[8,21]
24	Molybdenum	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[1,4,12] 2) Digestion, Inductively Coupled Plasma Method ^[5,12]
25	Nickel	1) Waste Extraction, Digestion, Flame Atomic Absorption Spectrometric Method ^[1,4,13] 2) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[1,4,12] 3) Digestion, Flame Atomic Absorption Spectrometric Method ^[5,13] 4) Digestion, Inductively Coupled Plasma Method ^[5,12]

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
26	<p>Polychlorinated Biphenyls</p> <ul style="list-style-type: none"> - Aroclor 1016 - Aroclor 1221 - Aroclor 1232 - Aroclor 1242 - Aroclor 1248 - Aroclor 1254 - Aroclor 1260 - 2-Chlorobiphenyl - 2,3-Dichlorobiphenyl - 2,2',5-Trichlorobiphenyl - 2,4',5-Trichlorobiphenyl - 2,2',3,5'-Tetrachlorobiphenyl - 2,2',5,5'-Tetrachlorobiphenyl - 2,3',4,4'-Tetrachlorobiphenyl - 2,2',3,4,5'-Pentachlorobiphenyl - 2,2',4,5,5'-Pentachlorobiphenyl - 2,3,3',4',6-Pentachlorobiphenyl - 2,2',3,4,4',5'-Hexachlorobiphenyl - 2,2',3,4,5,5'-Hexachlorobiphenyl - 2,2',3,5,5',6-Hexachlorobiphenyl - 2,2',4,4',5,5'-Hexachlorobiphenyl - 2,2',3,3',4,4',5-Heptachlorobiphenyl - 2,2',3,4,4',5,5'-Heptachlorobiphenyl - 2,2',3,4,4',5,6-Heptachlorobiphenyl - 2,2',3,4',5,5',6-Heptachlorobiphenyl - 2,2',3,3',4,4',5,6-Heptachlorobiphenyl - Nonachlorobiphenyl 	<p>1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method^[1,7,22]</p> <p>2) Ultrasonic Extraction, Gas Chromatographic Method^[8,22]</p>

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
27	Pentachlorophenol	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[1,7,24] 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[8,24]
28	pH	Electrometric Method ^[25,26]
29	Selenium	1) Waste Extraction, Digestion, Hydride Generation/Atomic Absorption Spectrometric Method ^[1,4,19] 2) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[1,4,12] 3) Digestion, Hydride Generation/Atomic Absorption Spectrometric Method ^[5,19] 4) Digestion, Inductively Coupled Plasma Method ^[5,12]
30	Silver	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[1,4,12] 2) Digestion, Inductively Coupled Plasma Method ^[5,12]
31	Thallium	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[1,4,12] 2) Digestion, Inductively Coupled Plasma Method ^[5,12]
32	Toxaphene	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method ^[1,7,21] 2) Ultrasonic Extraction, Gas Chromatographic Method ^[8,21]
33	Trichloroethylene	1) Waste Extraction, Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[1,10,23] 2) Waste Extraction, Equilibrium Headspace, Gas Chromatographic/Mass Spectrometric Method ^[1,9,23] 3) Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[11,23] 4) Equilibrium Headspace, Gas Chromatographic/Mass Spectrometric Method ^[9,23]
34	Vanadium	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[1,4,12] 2) Digestion, Inductively Coupled Plasma Method ^[5,12]

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
35	Zinc	1) Waste Extraction, Digestion, Flame Atomic Absorption Spectrometric Method ^[1,4,13] 2) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[1,4,12] 3) Digestion, Flame Atomic Absorption Spectrometric Method ^[5,15] 4) Digestion, Inductively Coupled Plasma Method ^[5,12]

เอกสารอ้างอิง

- กระทรวงอุตสาหกรรม. ประกาศกระทรวงอุตสาหกรรม, พ.ศ. 2566. เรื่อง การจัดการสิ่งปฏิกูลหรือวัสดุที่ไม่ใช้แล้ว.ราชกิจจานุเบกษา. 31 พฤษภาคม 2566. เล่มที่ 140 ตอนพิเศษ 126 ง.
- สมาคมวิศวกรรมสิ่งแวดล้อมแห่งประเทศไทย. คู่มือวิเคราะห์น้ำเสีย. พิมพ์ครั้งที่ 4. กรุงเทพฯ: เรือนแก้วการพิมพ์, 2547.
- APHA, AWWA, WEF. **Standard Methods for the Examination of Water and Wastewater**. 24th ed. Washington, DC: APHA, 2023.
- United States Environmental Protection Agency. **Test Methods for Evaluation Solid Waste Physical/Chemical Methods**. SW-846, 2014.
- United States Environmental Protection Agency. **Test Methods for Evaluation Solid Waste Physical/Chemical Methods. Acid Digestion of Sediments, Sludges, and Soils**. SW-846 Method 3050B, 1996.
- United States Environmental Protection Agency. **Test Methods for Evaluation Solid Waste Physical/Chemical Methods. Alkaline Digestion for Hexavalent Chromium**. SW-846 Method 3060A, 1996.
- United States Environmental Protection Agency. **Test Methods for Evaluation Solid Waste 3. Physical/Chemical Methods. Separatory Funnel Liquid-Liquid Extraction**. SW-846 Method 3510C, 1996.
- United States Environmental Protection Agency. **Test Methods for Evaluation Solid Waste Physical/Chemical Methods. Ultrasonic Extraction**. SW-846 Method 3550C, 2007.
- United States Environmental Protection Agency. **Test Methods for Evaluation Solid Waste Physical/Chemical Methods. Volatile Organic Compounds in Various Sample Matrices Using Equilibrium Headspace Analysis**. SW-846 Method 5021A, 2014.
- United States Environmental Protection Agency. **Test Methods for Evaluation Solid Waste Physical/Chemical Methods. Purge and Trap for Aqueous Samples**. SW-846 Method 5030C, 2003.
- United States Environmental Protection Agency. **Test Methods for Evaluation Solid Waste Physical/Chemical Methods. Closed System Purge and Trap and Extraction for Volatile Organics in Soil and Waste Sample**. SW-846 Method 5035A, 2000.

12. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Inductively Coupled Plasma-Optical Emission Spectrometry. SW-846 Method 6010D**, 2014.
13. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Flame Atomic Absorption Spectrophotometry. SW-846 Method 7000B**, 2007.
14. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Arsenic (Atomic Absorption, Gaseous Hydride). SW-846 Method 7061A**, 1992.
15. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Chromium, Hexavalent (Colorimetric). SW-846 Method 7196A**, 1992.
16. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Mercury in Liquid Waste (Manual Cold Vapor Technique). SW-846 Method 7470A**, 1994.
17. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Mercury in Solid or Semisolid Waste (Manual Cold-Vapor Technique). SW-846 Method 7471B**, 1998.
18. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Mercury in Solids and Solutions by Thermal Decomposition, Amalgamation, and Atomic Absorption Spectrophotometry. SW-846 Method 7473**, 2007.
19. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Selenium (Atomic Absorption, Borohydride Reduction). SW-846 Method 7742**, 1994.
20. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Nonhalogenated Organics Using GC/FID. SW-846 Method 8015D**, 2003.
21. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Organochlorine Pesticides by Gas Chromatography. SW-846 Method 8081B**, 2007.
22. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Polychlorinated Biphenyls (PCBs) by Gas Chromatography. SW-846 Method 8082A**, 2007.
23. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Volatile Organic Compounds by Gas Chromatography/Mass Spectrometry. SW-846 Method 8260D**, 2018.
24. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Semivolatile Organic Compounds by Gas Chromatography/Mass Spectrometry. SW-846 Method 8270E**, 2018.
25. United States...

25. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. pH Electrometric Measurement. SW-846 Method 9040C, 2004.

26. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. Soil and Waste pH. SW-846 Method 9045D, 2004. [REDACTED]



[REDACTED]
ดำเนินโดย



ที่ อก ๐๓๑๐(๑)/ ๑๖๙๑๘

กรมโรงงานอุตสาหกรรม
ถนนพระรามที่ ๖ แขวงทุ่งพญาไท
เขตราชเทวี กรุงเทพฯ ๑๐๕๐๐

๑๓ ธันวาคม ๒๕๖๖


เรื่อง เปลี่ยนแปลงบุคลากรของห้องปฏิบัติการวิเคราะห์

เรียน กรรมการผู้จัดการ บริษัท ยูไนเต็ท แอนนาลิสต์ แอนด์ เอ็นจิเนียริง คอนซัลแตนท์ จำกัด

อ้างถึง คำขอขึ้นทะเบียน/ต่ออายุ/เปลี่ยนแปลงบุคลากร และขณิศจาแนบของห้องปฏิบัติการวิเคราะห์เอกชน
ลงวันที่ ๗ พฤศจิกายน ๒๕๖๖

ตามหนังสือที่อ้างถึง บริษัท ยูไนเต็ท แอนนาลิสต์ แอนด์ เอ็นจิเนียริง คอนซัลแตนท์ จำกัด
ห้องปฏิบัติการวิเคราะห์เอกชน เลขทะเบียน ว-๑๔๕ สถานที่ตั้งเลขที่ ๓ ซอยอุดมสุข ๔๑ ถนนสุขุมวิท
แขวงบางจาก เขตพระโขนง กรุงเทพมหานคร ขอเปลี่ยนแปลงบุคลากรของห้องปฏิบัติการวิเคราะห์
ความละเอียดแจ้งแล้ว นั้น

กรมโรงงานอุตสาหกรรมพิจารณาแล้ว ให้เพิ่มเจ้าหน้าที่ประจำห้องปฏิบัติการวิเคราะห์
จำนวน ๖ ราย ได้แก่



อนึ่ง หนังสือฉบับนี้จะหมดอายุพร้อมหนังสือต่ออายุรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์
เอกชน คือในวันที่ ๒ กุมภาพันธ์ ๒๕๖๘ ทั้งนี้ สามารถยื่นคำขอผ่านระบบอิเล็กทรอนิกส์ได้ที่หน้าเว็บไซต์
กรมโรงงานอุตสาหกรรม

จึงเรียนมาเพื่อทราบ

ขอแสดงความนับถือ



ผู้อำนวยการกองวิจัยและเคอเมียมลพิษโรงงาน
นักวิชาการแผนอัตรากำลังกรมโรงงานอุตสาหกรรม



อำนาจถูกต้อง

กองวิจัยและเคอเมียมลพิษโรงงาน

กลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษและทะเบียนห้องปฏิบัติการ

โทร. ๐ ๒๔๓๐ ๖๓๑๒ ต่อ ๒๑๐๓-๕

โทรสาร ๐ ๒๔๓๐ ๖๓๑๒ ต่อ ๒๑๔๔

ไปรษณีย์อิเล็กทรอนิกส์ saraban@diw.mail.go.th



"อุตสาหกรรมก้าวไกล ประเทศไทยก้าวหน้า ร่วมกันพัฒนา อุตสาหกรรมสีเขียว"







ที่ อก ๐๓๓๐(๑)/ ๘๗๒๔

กรมโรงงานอุตสาหกรรม
ถนนพระรามที่ ๖ แขวงทุ่งพญาไท
เขตราชเทวี กรุงเทพฯ ๑๐๔๐๐

๒๕ พฤษภาคม ๒๕๖๖


เรื่อง เปลี่ยนแปลงบุคลากรของห้องปฏิบัติการวิเคราะห์

เรียน กรรมการผู้จัดการ บริษัท ยูโนเต็ด แอนนาลิสต์ แอนด์ เอ็นจิเนียริง คอนซัลแตนท์ จำกัด

อ้างถึง คำขอขึ้นทะเบียน/ต่ออายุ/เปลี่ยนแปลงบุคลากร และชนิดสารมลพิษของห้องปฏิบัติการวิเคราะห์เอกชน
ลงวันที่ ๑๖ พฤษภาคม ๒๕๖๖

ตามหนังสือที่อ้างถึง บริษัท ยูโนเต็ด แอนนาลิสต์ แอนด์ เอ็นจิเนียริง คอนซัลแตนท์ จำกัด
ห้องปฏิบัติการวิเคราะห์เอกชน เลขทะเบียน ว-๑๔๕ สถานที่ตั้งเลขที่ ๓ ซอยอุดมสุข ๔๑ ถนนสุขุมวิท แขวงบางจาก
เขตพระโขนง กรุงเทพมหานคร ขอเปลี่ยนแปลงบุคลากรของห้องปฏิบัติการวิเคราะห์ ความละเอียดแจ้งแล้ว นั้น


กรมโรงงานอุตสาหกรรมพิจารณาแล้ว มีความเห็นดังนี้



อนึ่ง หนังสือฉบับนี้จะหมดอายุพร้อมหนังสือต่ออายุรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์
เอกชน คือในวันที่ ๒ กุมภาพันธ์ ๒๕๖๘ ทั้งนี้ สามารถยื่นคำขอผ่านระบบอิเล็กทรอนิกส์ได้ที่หน้าเว็บไซต์
กรมโรงงานอุตสาหกรรม

จึงเรียนมาเพื่อทราบ

ขอแสดงความนับถือ



ผู้อำนวยการกองวิจัยและเตือนภัยมลพิษโรงงาน
ปฏิบัติการตามแผนปฏิบัติการโรงงานอุตสาหกรรม

UNITED ANALYST AND ENGINEERING
CONSULTANT COMPANY LIMITED

อำนาจถูกต้อง

กองวิจัยและเตือนภัยมลพิษโรงงาน

กลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษและทะเบียนห้องปฏิบัติการ

โทร. ๐ ๒๔๓๐ ๖๓๑๒ ต่อ ๒๑๐๓-๕

โทรสาร ๐ ๒๔๓๐ ๖๓๑๒ ต่อ ๒๑๔๔

ไปรษณีย์อิเล็กทรอนิกส์ saraban@diw.mail.go.th



“อุตสาหกรรมก้าวไกล ประเทศไทยก้าวหน้า ร่วมกันพัฒนา อุตสาหกรรมสีเขียว”







ที่ อก ๐๓๑๐(๑)/ ๒๐๒๘

กรมโรงงานอุตสาหกรรม
ถนนพระรามที่ ๖ แขวงทุ่งพญาไท
เขตราชเทวี กรุงเทพฯ ๑๐๕๐๐

๒๒ มีนาคม ๒๕๖๖

เรื่อง เปลี่ยนแปลงบุคลากรและสารมลพิษที่วิเคราะห์

เรียน กรรมการผู้จัดการ บริษัท ยูโนเด็ค แอนนาลิสต์ แอนด์ เอ็นจิเนียริง คอนซัลแตนท์ จำกัด


อ้างถึง คำขอขึ้นทะเบียน/ต่ออายุ/เปลี่ยนแปลงบุคลากร และชนิดสารมลพิษของห้องปฏิบัติการวิเคราะห์เอกชน
ลงวันที่ ๓๐ มกราคม ๒๕๖๖

สิ่งที่ส่งมาด้วย เอกสารแนบท้ายหนังสือเปลี่ยนแปลงบุคลากรและสารมลพิษที่วิเคราะห์

บริษัท ยูโนเด็ค แอนนาลิสต์ แอนด์ เอ็นจิเนียริง คอนซัลแตนท์ จำกัด จำนวน ๒ แผ่น

ตามหนังสือที่อ้างถึง บริษัท ยูโนเด็ค แอนนาลิสต์ แอนด์ เอ็นจิเนียริง คอนซัลแตนท์ จำกัด
ห้องปฏิบัติการวิเคราะห์เอกชน เลขทะเบียน ว-๑๔๕๕ สถานที่ตั้งเลขที่ ๓ ซอยอุดมสุข ๔๑ ถนนสุขุมวิท
แขวงบางจาก เขตพระโขนง กรุงเทพมหานคร ขอเปลี่ยนแปลงบุคลากรและสารมลพิษที่วิเคราะห์
ความละเอียดแจ้งแล้ว นั้น

กรมโรงงานอุตสาหกรรมพิจารณาแล้ว มีความเห็นดังนี้



๓. ให้เพิ่มขอบข่ายสารมลพิษที่วิเคราะห์ในดิน ตามสิ่งที่ส่งมาด้วย

UAE
UNITED ANALYST AND ENGINEERING
CONSULTANT COMPANY LIMITED

ดำเนินการถูกต้อง

อนึ่ง...

อนึ่ง หนังสือฉบับนี้จะหมดอายุพร้อมหนังสือต่ออายุรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน
ที่ อก ๐๓๑๐(ด)/๑๘๗๙ ลงวันที่ ๙ กุมภาพันธ์ ๒๕๖๕ คือในวันที่ ๒ กุมภาพันธ์ ๒๕๖๘ ทั้งนี้ สามารถยื่นคำขอ
ผ่านระบบอิเล็กทรอนิกส์ได้ที่หน้าเว็บไซต์กรมโรงงานอุตสาหกรรม ตาม QR Code ห้าหนังสือฉบับนี้

จึงเรียนมาเพื่อทราบ

ขอแสดงความนับถือ



ผู้อำนวยการกองวิจัยและเตือนภัยมลพิษโรงงาน
ปฏิบัติการตามหนังสือกรมโรงงานอุตสาหกรรม



ยื่นคำขอผ่านระบบอิเล็กทรอนิกส์

กองวิจัยและเตือนภัยมลพิษโรงงาน

กลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษและทะเบียนห้องปฏิบัติการ

โทร. ๐ ๒๕๓๐ ๒๓๑๒ ต่อ ๒๑๐๓-๕ โทรสาร ๐ ๒๕๓๐ ๖๓๑๒ ต่อ ๑๑๔๙

ไปรษณีย์อิเล็กทรอนิกส์ saraban@diw.mail.go.th

UAE

UNITED ANALYST AND ENGINEERING
CONSULTANT COMPANY LIMITED

ดำเนินาถูกต้อง



เอกสารแนบท้ายหนังสือเปลี่ยนแปลงบุคลากรและสารมลพิษที่วิเคราะห์

บริษัท ยูนิเทค แอนนาลิซิส แอนด์ เอ็นจิเนียริง คอนซัลแตนท์ จำกัด

เลขทะเบียน ว-๑๔๕

ที่ อก ๐๓๑๐(๑)/ ๖ ๐ ๒ ๘

ลงวันที่ ๒๒ มีนาคม ๒๕๖๖

ขอขยายสารมลพิษที่ได้รับขึ้นทะเบียนจากกรมโรงงานอุตสาหกรรม จำนวน ๑๖ รายการ

เดิม จำนวน 16 รายการ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
1	Benzene	Equilibrium Headspace, Gas Chromatographic/ Mass Spectrometric Method ^[1,2]
2	Carbon tetrachloride	Equilibrium Headspace, Gas Chromatographic/ Mass Spectrometric Method ^[1,2]
3	1,2-Dichloroethane	Equilibrium Headspace, Gas Chromatographic/ Mass Spectrometric Method ^[1,2]
4	1,1-Dichloroethylene	Equilibrium Headspace, Gas Chromatographic/ Mass Spectrometric Method ^[1,2]
5	cis-1,2-Dichloroethylene	Equilibrium Headspace, Gas Chromatographic/ Mass Spectrometric Method ^[1,2]
6	trans-1,2-Dichloroethylene	Equilibrium Headspace, Gas Chromatographic/ Mass Spectrometric Method ^[1,2]
7	Ethylbenzene	Equilibrium Headspace, Gas Chromatographic/ Mass Spectrometric Method ^[1,2]
8	Methylene chloride	Equilibrium Headspace, Gas Chromatographic/ Mass Spectrometric Method ^[1,2]
9	Styrene	Equilibrium Headspace, Gas Chromatographic/ Mass Spectrometric Method ^[1,2]
10	Tetrachloroethylene	Equilibrium Headspace, Gas Chromatographic/ Mass Spectrometric Method ^[1,2]
11	Toluene	Equilibrium Headspace, Gas Chromatographic/ Mass Spectrometric Method ^[1,2]
12	Trichloroethylene	Equilibrium Headspace, Gas Chromatographic/ Mass Spectrometric Method ^[1,2]
13	m-Xylene	Equilibrium Headspace, Gas Chromatographic/ Mass Spectrometric Method ^[1,2]
14	o-Xylene	Equilibrium Headspace, Gas Chromatographic/ Mass Spectrometric Method ^[1,2]
15	p-Xylene	Equilibrium Headspace, Gas Chromatographic/ Mass Spectrometric Method ^[1,2]
16	Xylene (Total)	Equilibrium Headspace, Gas Chromatographic/ Mass Spectrometric Method ^[1,2]

เอกสารอ้างอิง...

เอกสารอ้างอิง

1. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. Volatile Organic Compounds in Various Sample Matrices Using Equilibrium Headspace Analysis. SW-846 Method 5021A, 2014.
2. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. Volatile Organic Compounds by Gas Chromatography/Mass Spectrometry. SW-846 Method 8260D, 2018. [REDACTED]





ที่ อก ๐๓๑๐(๑)/ ๑๕๕๕๓

กรมโรงงานอุตสาหกรรม
ถนนพระรามที่ ๖ แขวงทุ่งพญาไท
เขตราชเทวี กรุงเทพฯ ๑๐๕๐๐

๒๕ ตุลาคม ๒๕๖๕


เรื่อง เปลี่ยนแปลงบุคลากรของห้องปฏิบัติการวิเคราะห์

เรียน กรรมการผู้จัดการ บริษัท ยูไนเต็ด แอนนาลิสต์ แอนด์ เอ็นจิเนียริง คอนซัลแตนท์ จำกัด

อ้างถึง คำขอขึ้นทะเบียน/ต่ออายุ/เปลี่ยนแปลงบุคลากร และชนิดสารมลพิษของห้องปฏิบัติการวิเคราะห์เอกชน
ลงวันที่ ๑๘ ตุลาคม ๒๕๖๕

ตามหนังสือที่อ้างถึง บริษัท ยูไนเต็ด แอนนาลิสต์ แอนด์ เอ็นจิเนียริง คอนซัลแตนท์ จำกัด
ห้องปฏิบัติการวิเคราะห์เอกชน เลขทะเบียน ว-๑๔๕ สถานที่ตั้งเลขที่ ๓ ซอยอุดมสุข ๔๑ ถนนสุขุมวิท แขวงบางจาก
เขตพระโขนง กรุงเทพมหานคร ขอเปลี่ยนแปลงบุคลากรของห้องปฏิบัติการวิเคราะห์ ความละเอียดแจ้งแล้ว นั้น

กรมโรงงานอุตสาหกรรมพิจารณาแล้ว มีความเห็นดังนี้




CONSULTANT COMPANY LIMITED

อนึ่ง หนังสือฉบับนี้จะหมดอายุพร้อมหนังสือต่ออายุรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน
ที่ อก ๐๓๑๐(๑)/๑๘๗๙ ลงวันที่ ๙ กุมภาพันธ์ ๒๕๖๕ คือในวันที่ ๒ กุมภาพันธ์ ๒๕๖๘ ทั้งนี้ สามารถยื่นคำขอ
ผ่านระบบอิเล็กทรอนิกส์ได้ที่หน้าเว็บไซต์กรมโรงงานอุตสาหกรรม ตาม QR Code หายหนังสือฉบับนี้

จึงเรียนมาเพื่อทราบ

ขอแสดงความนับถือ



ผู้อำนวยการกองวิจัยและเตือนภัยมลพิษโรงงาน
ปฏิบัติราชการแทนอธิบดีกรมโรงงานอุตสาหกรรม



ยื่นคำขอผ่านระบบอิเล็กทรอนิกส์

กองวิจัยและเตือนภัยมลพิษโรงงาน

กลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษและทะเบียนห้องปฏิบัติการ


โทร. ๐ ๒๔๓๐ ๖๓๑๒ ต่อ ๒๑๐๓-๕

โทรสาร ๐ ๒๔๓๐ ๖๓๑๒ ต่อ ๒๑๔๙

ไปรษณีย์อิเล็กทรอนิกส์ saraban@diw.mail.go.th



ดำเนินตามกฎหมาย



“อุตสาหกรรมก้าวไกล ประเทศไทยก้าวหน้า ร่วมกันพัฒนา อุตสาหกรรมสีเขียว”





ที่ อก ๐๓๑๐(๑)/ ๑๒ ๑๗ ๓

กรมโรงงานอุตสาหกรรม
ถนนพระรามที่ ๖ แขวงทุ่งพญาไท
เขตราชเทวี กรุงเทพฯ ๑๐๕๐๐


๐ ๑ กันยายน ๒๕๖๕

เรื่อง เปลี่ยนแปลงบุคลากรของห้องปฏิบัติการวิเคราะห์

เรียน กรรมการผู้จัดการ บริษัท ยูโนเด็ค แอนนาลิสต์ แอนด์ เอ็นจิเนียริง คอนซัลแตนท์ จำกัด

อ้างถึง คำขอขึ้นทะเบียน/ต่ออายุ/เปลี่ยนแปลงบุคลากร และชนิดสารมลพิษของห้องปฏิบัติการวิเคราะห์เอกชน
ลงวันที่ ๒๒ สิงหาคม ๒๕๖๕

ตามหนังสือที่อ้างถึง บริษัท ยูโนเด็ค แอนนาลิสต์ แอนด์ เอ็นจิเนียริง คอนซัลแตนท์ จำกัด
ห้องปฏิบัติการวิเคราะห์เอกชน เลขทะเบียน ว-๑๕๕ สถานที่ตั้งเลขที่ ๓ ซอยอุดมสุข ๕๑ ถนนสุขุมวิท แขวงบางจาก
เขตพระโขนง กรุงเทพมหานคร ขอเปลี่ยนแปลงบุคลากรของห้องปฏิบัติการวิเคราะห์ ความละเอียดแจ้งแล้ว นั้น
กรมโรงงานอุตสาหกรรมพิจารณาแล้ว มีความเห็นดังนี้



CONSULTANT COMPANY LIMITED

อนึ่ง หนังสือฉบับนี้...

อนึ่ง หนังสือฉบับนี้จะหมดอายุพร้อมหนังสือต่ออายุรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน
ที่ กก ๐๓๑๐(๑)/๑๘๗๙ ลงวันที่ ๙ กุมภาพันธ์ ๒๕๖๕ คือในวันที่ ๒ กุมภาพันธ์ ๒๕๖๘ ทั้งนี้ สามารถยื่นคำขอ
ผ่านระบบอิเล็กทรอนิกส์ได้ที่หน้าเว็บไซต์กรมโรงงานอุตสาหกรรม ตาม QR Code ท้ายหนังสือฉบับนี้

จึงเรียนมาเพื่อทราบ

ขอแสดงความนับถือ



ผู้อำนวยการกองวิจัยและพัฒนาผลิตภัณฑ์โรงงาน
ปฏิบัติราชการแทนอธิบดีกรมโรงงานอุตสาหกรรม



ยื่นคำขอผ่านระบบอิเล็กทรอนิกส์

กองวิจัยและพัฒนาผลิตภัณฑ์โรงงาน
กลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบผลิตภัณฑ์และทะเบียนห้องปฏิบัติการ
โทร. ๐ ๒๔๓๐ ๖๓๑๒ ต่อ ๒๑๐๓-๕
โทรสาร ๐ ๒๔๓๐ ๖๓๑๒ ต่อ ๒๑๔๙
ไปรษณีย์อิเล็กทรอนิกส์ saraban@diw.mail.go.th



ดำเนินการถูกต้อง



“อุตสาหกรรมก้าวไกล ประเทศไทยก้าวหน้า ร่วมกันพัฒนา อุตสาหกรรมสีเขียว”



ที่ อก ๐๓๑๐(๑)/ ๔๗๘ ๗



กรมโรงงานอุตสาหกรรม
ถนนพระรามที่ ๖ แขวงทุ่งพญาไท
เขตราชเทวี กรุงเทพฯ ๑๐๕๐๐

๒๑ เมษายน ๒๕๖๕


เรื่อง เปลี่ยนแปลงบุคลากรของห้องปฏิบัติการวิเคราะห์

เรียน กรรมการผู้จัดการ บริษัท ยูไนเตค แอนนาลิสต์ แอนด์ เอ็นจิเนียริง คอนซัลแตนท์ จำกัด

อ้างถึง คำขอขึ้นทะเบียน/ต่ออายุ/เปลี่ยนแปลงบุคลากร และชนิดสารมลพิษของห้องปฏิบัติการวิเคราะห์เอกชน
ลงวันที่ ๓๐ มีนาคม ๒๕๖๕

ตามหนังสือที่อ้างถึง บริษัท ยูไนเตค แอนนาลิสต์ แอนด์ เอ็นจิเนียริง คอนซัลแตนท์ จำกัด
ห้องปฏิบัติการวิเคราะห์เอกชน เลขทะเบียน ว-๑๔๕ สถานที่ตั้งเลขที่ ๓ ซอยอุดมสุข ถนนสุขุมวิท แขวงบางจาก
เขตพระโขนง กรุงเทพมหานคร ขอเปลี่ยนแปลงบุคลากรของห้องปฏิบัติการวิเคราะห์ ความละเอียดแจ้งแล้ว นั้น


กรมโรงงานอุตสาหกรรมพิจารณาแล้ว มีความเห็นดังนี้



อนึ่ง หนังสือฉบับนี้จะหมดอายุพร้อมหนังสือต่ออายุรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน
ที่ อก ๐๓๑๐(๑)/๑๘๘๙ ลงวันที่ ๙ กุมภาพันธ์ ๒๕๖๕ คือในวันที่ ๒ กุมภาพันธ์ ๒๕๖๘ ทั้งนี้ สามารถยื่นคำขอ
ผ่านระบบอิเล็กทรอนิกส์ได้ที่หน้าเว็บไซต์กรมโรงงานอุตสาหกรรม ตาม QR Code ท้ายหนังสือฉบับนี้

จึงเรียนมาเพื่อทราบ

ขอแสดงความนับถือ



ผู้อำนวยการกองวิจัยและเตือนภัยมลพิษโรงงาน
ปฏิบัติการตามหนังสือกรมโรงงานอุตสาหกรรม



ยื่นคำขอผ่านระบบอิเล็กทรอนิกส์

กองวิจัยและเตือนภัยมลพิษโรงงาน

กลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษและทะเบียนห้องปฏิบัติการ

โทร. ๐ ๒๕๓๐ ๖๓๑๒ ต่อ ๒๑๐๓-๕ โทรสาร ๐ ๒๕๓๐ ๖๓๑๒ ต่อ ๒๑๙๓

ไปรษณีย์อิเล็กทรอนิกส์ saraban@diw.mail.go.th



ดำเนินการถูกต้อง



“อุตสาหกรรมก้าวไกล ประเทศไทยก้าวหน้า ร่วมกันพัฒนา อุตสาหกรรมสีเขียว”







ที่ อภ ๐๓๑๐(๑)/ ๑๘๗ ๙

กรมโรงงานอุตสาหกรรม
ถนนพระรามที่ ๖ แขวงทุ่งพญาไท
เขตราชเทวี กรุงเทพฯ ๑๐๔๐๐

๐ ๙ กุมภาพันธ์ ๒๕๖๕

เรื่อง ต่ออายุหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน

เรียน กรรมการผู้จัดการ บริษัท ยูโนเด็ค แอนนาลิสต์ แอนด์ เอ็นจิเนียริง คอนซัลแตนท์ จำกัด

อ้างถึง คำขอขึ้นทะเบียน/ต่ออายุ/เปลี่ยนแปลงบุคลากร และชนิดสารมลพิษของห้องปฏิบัติการวิเคราะห์เอกชน
ลงวันที่ ๒๗ ธันวาคม ๒๕๖๔

สิ่งที่ส่งมาด้วย ๑. รายชื่อผู้ควบคุมดูแลห้องปฏิบัติการวิเคราะห์ จำนวน ๔๐ ราย
๒. รายชื่อเจ้าหน้าที่ประจำห้องปฏิบัติการวิเคราะห์ จำนวน ๑๐๖ ราย
๓. ขอบข่ายสารมลพิษที่ได้รับขึ้นทะเบียนจากกรมโรงงานอุตสาหกรรม

ตามหนังสือที่อ้างถึง บริษัท ยูโนเด็ค แอนนาลิสต์ แอนด์ เอ็นจิเนียริง คอนซัลแตนท์ จำกัด
ขอต่ออายุหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน เลขทะเบียน ว-๑๔๕ สถานที่ตั้งเลขที่ ๓
ซอยอุดมสุข ๔๑ ถนนสุขุมวิท แขวงบางจาก เขตพระโขนง กรุงเทพมหานคร ต่อกรมโรงงานอุตสาหกรรม นั้น

กรมโรงงานอุตสาหกรรมพิจารณาแล้ว ให้บริษัท ยูโนเด็ค แอนนาลิสต์ แอนด์ เอ็นจิเนียริง
คอนซัลแตนท์ จำกัด ต่ออายุหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน โดยมีองค์ประกอบดังนี้
ก. ผู้ควบคุมดูแลห้องปฏิบัติการวิเคราะห์ จำนวน ๔๐ ราย ตามสิ่งที่ส่งมาด้วย ๑
ข. เจ้าหน้าที่ประจำห้องปฏิบัติการวิเคราะห์ จำนวน ๑๐๖ ราย ตามสิ่งที่ส่งมาด้วย ๒
ค. ขอบข่ายสารมลพิษที่ได้รับขึ้นทะเบียนให้วิเคราะห์ในน้ำเสีย น้ำใต้ดิน อากาศเสีย สิ่งปฏิกูล
หรือวัสดุที่ไม่ใช้แล้ว และดิน ตามสิ่งที่ส่งมาด้วย ๓

หนังสือฉบับนี้จะหมดอายุในวันที่ ๒ กุมภาพันธ์ ๒๕๖๘ หากประสงค์จะต่ออายุหนังสือ
รับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน ให้ยื่นคำขอต่ออายุพร้อมเอกสารประกอบคำขอต่อ
กรมโรงงานอุตสาหกรรมภายใน ๓๐ วัน ก่อนวันสิ้นอายุของหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน
ทั้งนี้ สามารถยื่นคำขอผ่านระบบอิเล็กทรอนิกส์ได้ที่หน้าเว็บไซต์กรมโรงงานอุตสาหกรรม ตาม QR Code ห้าง
หนังสือฉบับนี้

จึงเรียนมาเพื่อทราบ

ขอแสดงความนับถือ

ผู้อำนวยการและตัวแทนของกรมโรงงาน
อุตสาหกรรม กรุงเทพมหานคร

UNITED ANALYST AND ENGINEERING
CONSULTANT COMPANY LIMITED

ไดนามิกคอก

กองวิจัยและเตือนภัยมลพิษโรงงาน

กลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษและทะเบียนห้องปฏิบัติการ

โทร. ๐ ๒๔๓๐ ๖๓๑๒ ต่อ ๒๑๐๓-๕


โทรสาร ๐ ๒๔๓๐ ๖๓๑๒ ต่อ ๒๑๙๙

ไปรษณีย์อิเล็กทรอนิกส์ saraban@diw.gmail.go.th

เอกสารแนบท้ายหนังสือรับต่ออายุขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน
บริษัท ยูไนเต็ด แอนนาลิสต์ แอนด์ เอ็นจิเนียริง คอนซัลแตนท์ จำกัด เลขทะเบียน ว-๑๔๕
ที่ อก ๐๓๑๐(๑)/ ๑๘๗๙ ลงวันที่ ๐๙ กุมภาพันธ์ ๒๕๖๕

ก. ผู้ควบคุมดูแลห้องปฏิบัติการวิเคราะห์ จำนวน ๕๐ ราย





ผู้อำนวยการกองวิจัยและเค่อนภัยพิบัติโรงงาน
ปฏิบัติราชการหนอยบังคับกรมโรงงานอุตสาหกรรม

กรมโรงงานอุตสาหกรรม
กระทรวงอุตสาหกรรม
เลขที่ ๑๒๓๔๕๖๗๘
กรุงเทพฯ ๑๐๐๐๐

UAE
UNITED ANALYST AND ENGINEERING
CONSULTANT COMPANY LIMITED




ดำเนินาอกตอง


เอกสารแนบท้ายหนังสือรับต่ออายุขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกสาร


บริษัท ยูไนเต็ด แอนนาลิสต์ แอนด์ เอ็นจิเนียริง คอนซัลแตนท์ จำกัด เลขทะเบียน ว-๑๕๕

ที่ อก ๐๓๑๐(๑)/ ๑๘๗ ๕ ลงวันที่ ๐๕ กุมภาพันธ์ ๒๕๖๕

ข. เจ้าหน้าที่ประจำห้องปฏิบัติการวิเคราะห์ จำนวน ๑๐๖ ราย







เอกสารแนบท้ายหนังสือรับต่ออายุขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน

บริษัท ยูโนเด็ค แอนนาไลส์ แอนด์ เอ็นจิเนียริง คอนซัลแตนท์ จำกัด เลขทะเบียน ว-๑๔๕

ที่ อก ๐๓๑๐(๑)/ ๓๘๗๕ ลงวันที่ ๐๙ กุมภาพันธ์ ๒๕๖๕

ขอขยายสารมลพิษที่ได้รับขึ้นทะเบียนจากกรมโรงงานอุตสาหกรรม จำนวน ๓๕๗ รายการ

น้ำเสีย จำนวน 46 รายการ

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
1	Aldrin	Liquid-Liquid Extraction, Gas Chromatographic Method ^[4]
2	Arsenic	1) Digestion, Hydride Generation/Atomic Absorption Spectrometric Method ^[4] 2) Digestion, Inductively Coupled Plasma Method ^[4]
3	Barium	Digestion, Inductively Coupled Plasma Method ^[4]
4	α -BHC	Liquid-Liquid Extraction, Gas Chromatographic Method ^[4]
5	β -BHC	Liquid-Liquid Extraction, Gas Chromatographic Method ^[4]
6	δ -BHC	Liquid-Liquid Extraction, Gas Chromatographic Method ^[4]
7	γ -BHC	Liquid-Liquid Extraction, Gas Chromatographic Method ^[4]
8	Biochemical Oxygen Demand	1) 5-Day BOD Test, Azide Modification Method ^[4] 2) 5-Day BOD Test, Membrane Electrode Method ^[4]
9	Cadmium	1) Digestion, Direct Air-Acetylene Flame Method ^[4] 2) Digestion, Electrothermal Atomic Absorption Spectrometric Method ^[4] 3) Digestion, Inductively Coupled Plasma Method ^[4]
10	Chemical Oxygen Demand	1) Closed Reflux, Titrimetric Method ^[4] 2) Closed Reflux, Colorimetric Method ^[4] 3) Open Reflux, Titrimetric Method ^[4]
11	Chlordane	Liquid-Liquid Extraction, Gas Chromatographic Method ^[4]
12	Chromium	1) Digestion, Direct Air Acetylene Flame Method ^[4] 2) Digestion, Electrothermal Atomic Absorption Spectrometric Method ^[4] 3) Digestion, Inductively Coupled Plasma Method ^[4]
13	Color	ADMI Weighted-Ordinate Spectrophotometric Method ^[4]
14	Copper	1) Digestion, Direct Air-Acetylene Flame Method ^[4] 2) Digestion, Electrothermal Atomic Absorption Spectrometric Method ^[4] 3) Digestion, Inductively Coupled Plasma Method ^[4]
15	Cyanide	1) Distillation, Colorimetric Method ^[4] 2) Flow Injection Analysis Method ^[4]

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
16	o,p'-DDT	Liquid-Liquid Extraction, Gas Chromatographic Method ⁽⁴⁾
17	4,4'-DDD	Liquid-Liquid Extraction, Gas Chromatographic Method ⁽⁴⁾
18	4,4'-DDE	Liquid-Liquid Extraction, Gas Chromatographic Method ⁽⁴⁾
19	4,4'-DDT	Liquid-Liquid Extraction, Gas Chromatographic Method ⁽⁴⁾
20	Dieldrin	Liquid-Liquid Extraction, Gas Chromatographic Method ⁽⁴⁾
21	Endosulfan I	Liquid-Liquid Extraction, Gas Chromatographic Method ⁽⁴⁾
22	Endosulfan II	Liquid-Liquid Extraction, Gas Chromatographic Method ⁽⁴⁾
23	Endosulfan sulfate	Liquid-Liquid Extraction, Gas Chromatographic Method ⁽⁴⁾
24	Endrin	Liquid-Liquid Extraction, Gas Chromatographic Method ⁽⁴⁾
25	Endrin aldehyde	Liquid-Liquid Extraction, Gas Chromatographic Method ⁽⁴⁾
26	Formaldehyde	Distillation, Colorimetric Method ⁽³⁾
27	Free Chlorine	1) Iodometric Method ⁽⁴⁾ 2) DPD Ferrous Titrimetric Method ⁽¹⁾
28	Heptachlor	Liquid-Liquid Extraction, Gas Chromatographic Method ⁽⁴⁾
29	Heptachlor Epoxide	Liquid-Liquid Extraction, Gas Chromatographic Method ⁽⁴⁾
30	Hexavalent Chromium	1) Colorimetric Method ⁽⁴⁾ 2) Extraction, Direct Air-Acetylene Flame Method ⁽⁴⁾
31	Lead	1) Digestion, Direct Air-Acetylene Flame Method ⁽⁴⁾ 2) Digestion, Electrothermal Atomic Absorption Spectrometric Method ⁽⁴⁾ 3) Digestion, Inductively Coupled Plasma Method ⁽⁴⁾
32	Manganese	1) Digestion, Direct Air-Acetylene Flame Method ⁽⁴⁾ 2) Digestion, Electrothermal Atomic Absorption Spectrometric Method ⁽⁴⁾ 3) Digestion, Inductively Coupled Plasma Method ⁽⁴⁾
33	Mercury	Digestion, Cold-Vapor Atomic Absorption Spectrometric Method ⁽⁴⁾
34	Methoxychlor	Liquid-Liquid Extraction, Gas Chromatographic Method ⁽⁴⁾
35	Nickel	1) Digestion, Direct Air-Acetylene Flame Method ⁽⁴⁾ 2) Digestion, Electrothermal Atomic Absorption Spectrometric Method ⁽⁴⁾ 3) Digestion, Inductively Coupled Plasma Method ⁽⁴⁾

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
36	Oil & Grease	1) Liquid-Liquid, Partition-Gravimetric Method ^[4] 2) Soxhlet Extraction Method ^[4]
37	pH	Electrometric Method ^[4]
38	Phenols	1) Distillation, Chloroform Extraction Method ^[4] 2) Distillation, Direct Photometric Method ^[4]
39	Selenium	1) Digestion, Hydride Generation/Atomic Absorption Spectrometric Method ^[4] 2) Digestion, inductively Coupled Plasma Method ^[4]
40	Sulfide	1) Iodometric Method ^[4] 2) Methylene Blue Method ^[4]
41	Temperature	Laboratory and Field Methods ^[4]
42	Total Dissolved Solids	Dried at 180 °C ^[4]
43	Total Kjeldahl Nitrogen	Semi-Micro-Kjeldahl Method ^[4]
44	Total Suspended Solids	Dried at 103-105 °C ^[4]
45	Trivalent Chromium	1) Digestion, Direct Air-Acetylene Flame Method; Colorimetric Method; Calculation ^[4] 2) Digestion, Inductively Coupled Plasma Method; Colorimetric Method; Calculation ^[4]
46	Zinc	1) Digestion, Direct Air-Acetylene Flame Method ^[4] 2) Digestion, Electrothermal Atomic Absorption Spectrometric Method ^[4] 3) Digestion, Inductively Coupled Plasma Method ^[4]

น้ำใต้ดิน จำนวน 126 รายการ

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
1	Acenaphthene	1) Liquid-Liquid Extraction, Gas Chromatographic Method ^[4] 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
2	Acetone	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ^[4]
3	Aldrin	1) Liquid-Liquid Extraction, Gas Chromatographic Method ^[4] 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
4	Anthracene	1) Liquid-Liquid Extraction, Gas Chromatographic Method ⁽⁴⁾ 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
5	Antimony	Digestion, Inductively Coupled Plasma Method ⁽⁴⁾
6	Arsenic	1) Digestion, Hydride Generation/Atomic Absorption Spectrometric Method ⁽⁴⁾ 2) Digestion, Inductively Coupled Plasma Method ⁽⁴⁾
7	Atrazine	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
8	Barium	1) Digestion, Electrothermal Atomic Absorption Spectrometric Method ⁽⁴⁾ 2) Digestion, Inductively Coupled Plasma Method ⁽⁴⁾
9	Benz(a)anthracene	1) Liquid-Liquid Extraction, Gas Chromatographic Method ⁽⁴⁾ 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
10	Benzene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
11	Benzo(b)fluoranthene	1) Liquid-Liquid Extraction, Gas Chromatographic Method ⁽⁴⁾ 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
12	Benzo(k)fluoranthene	1) Liquid-Liquid Extraction, Gas Chromatographic Method ⁽⁴⁾ 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
13	Benzoic acid	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
14	Benzo(a)pyrene	1) Liquid-Liquid Extraction, Gas Chromatographic Method ⁽⁴⁾ 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
15	Benzo(g,h,i)perylene	1) Liquid-Liquid Extraction, Gas Chromatographic Method ^[4] 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
16	Beryllium	Digestion, Inductively Coupled Plasma Method ^[4]
17	Bis(2-chloroethyl)ether	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
18	Bis(2-ethylhexyl)phthalate	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
19	Bromodichloromethane	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ^[1]
20	Bromoform	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ^[4]
21	Butanol	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ^[4]
22	Butyl benzyl phthalate	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
23	Cadmium	1) Digestion, Direct Air-Acetylene Flame Method ^[4] 2) Digestion, Electrothermal Atomic Absorption Spectrometric Method ^[4] 3) Digestion, Inductively Coupled Plasma Method ^[4]
24	Carbazole	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
25	Carbon disulfide	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ^[4]
26	Carbon tetrachloride	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ^[1]
27	Chlordane	1) Liquid-Liquid Extraction, Gas Chromatographic Method ^[4] 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
28	p-Chloroaniline	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
29	Chlorobenzene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ^[4]

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
30	Chlorodibromomethane	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ^[4]
31	Chloroform	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ^[1]
32	2-Chlorophenol	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
33	Chromium	1) Digestion, Direct Air-Acetylene Flame Method ^[4] 2) Digestion, Electrothermal Atomic Absorption Spectrometric Method ^[4] 3) Digestion, Inductively Coupled Plasma Method ^[4]
34	Chromium (III)	1) Digestion, Direct Air-Acetylene Flame Method; Colorimetric Method; Calculation ^[4] 2) Digestion, Inductively Coupled Plasma Method; Colorimetric Method; Calculation ^[4]
35	Chromium (VI)	1) Colorimetric Method ^[4] 2) Extraction, Air-Acetylene Flame Method ^[4]
36	Chrysene	1) Liquid-Liquid Extraction, Gas Chromatographic Method ^[4] 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
37	Cyanide	Distillation, Colorimetric Method ^[4]
38	2,4-D	Liquid-Liquid Extraction, Gas Chromatographic Method ^[4]
39	DDD	1) Liquid-Liquid Extraction, Gas Chromatographic Method ^[4] 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
40	DDE	1) Liquid-Liquid Extraction, Gas Chromatographic Method ^[4] 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
41	DDT	1) Liquid-Liquid Extraction, Gas Chromatographic Method ^[4] 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
42	Dibenz(a,h)anthracene	1) Liquid-Liquid Extraction, Gas Chromatographic Method ^[4] 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
43	Di-n-butyl phthalate	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
44	1,2-Dichlorobenzene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ^[4]
45	1,3-Dichlorobenzene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ^[4]
46	1,4-Dichlorobenzene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ^[4]
47	3,3'-Dichlorobenzidine	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
48	1,1-Dichloroethane	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ^[4]
49	1,2-Dichloroethane	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ^[4]
50	1,1-Dichloroethylene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ^[4]
51	cis-1,2-Dichloroethylene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ^[4]
52	trans-1,2-Dichloroethylene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ^[4]
53	2,4-Dichlorophenol	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
54	1,2-Dichloropropane	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ^[4]
55	1,3-Dichloropropane	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ^[4]
56	1,3-Dichloropropene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ^[4]
57	Dieldrin	1) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4] 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
58	Diethyl phthalate	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
59	2,4-Dimethylphenol	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
60	2,4-Dinitrophenol	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
61	2,4-Dinitrotoluene	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
62	2,6-Dinitrotoluene	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
63	Di-n-Octyl phthalate	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
64	Endosulfan	1) Liquid-Liquid Extraction, Gas Chromatographic Method ^[4] 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
65	Endrin	1) Liquid-Liquid Extraction, Gas Chromatographic Method ^[4] 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
66	Ethylbenzene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ^[4]
67	Fluoranthene	1) Liquid-Liquid Extraction, Gas Chromatographic Method ^[4] 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
68	Fluorene	1) Liquid-Liquid Extraction, Gas Chromatographic Method ^[4] 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
69	Heptachlor	1) Liquid-Liquid Extraction, Gas Chromatographic Method ^[4] 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
70	Heptachlor epoxide	1) Liquid-Liquid Extraction, Gas Chromatographic Method ^[4] 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
71	Hexachlorobenzene	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
72	Hexachloro-1,3-butadiene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ^[4]
73	n-Hexane	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ^[4]
74	α -HCH	1) Liquid-Liquid Extraction, Gas Chromatographic Method ^[4] 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
75	β -HCH	1) Liquid-Liquid Extraction, Gas Chromatographic Method ^[4] 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
76	γ -HCH	1) Liquid-Liquid Extraction, Gas Chromatographic Method ^[4] 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
77	Hexachlorocyclopentadiene	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
78	Hexachloroethane	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
79	Indeno(1,2,3-cd)pyrene	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
80	Isophorone	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
81	Lead	1) Digestion, Direct Air-Acetylene Flame Method ^[4] 2) Digestion, Electrothermal Atomic Absorption Spectrometric Method ^[4] 3) Digestion, Inductively Coupled Plasma Atomic Emission Spectrometric Method ^[4]

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
82	Manganese	1) Digestion, Direct Air-Acetylene Flame Method ^[4] 2) Digestion, Electrothermal Atomic Absorption Spectrometric Method ^[4] 3) Digestion, Inductively Coupled Plasma Method ^[4]
83	Mercury	Digestion, Cold-Vapor Atomic Absorption Spectrometric Method ^[4]
84	Methanol	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ^[4]
85	Methoxychlor	Liquid-Liquid Extraction, Gas Chromatographic Method ^[4]
86	Methyl bromide	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ^[4]
87	Methylene chloride	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ^[4]
88	2-Methylphenol	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
89	2-Methylnaphthalene	1) Liquid-Liquid Extraction, Gas Chromatographic Method ^[4] 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
90	Methyl tert-butyl ether	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ^[4]
91	Naphthalene	1) Liquid-Liquid Extraction, Gas Chromatographic Method ^[4] 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
92	Nickel	1) Digestion, Direct Air-Acetylene Flame Method ^[4] 2) Digestion, Electrothermal Atomic Absorption Spectrometric Method ^[4] 3) Digestion, Inductively Coupled Plasma Method ^[4]
93	Nitrobenzene	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
94	N-Nitrosodiphenylamine	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
95	N-Nitrosodi-n-propylamine	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
96	Polychlorinated Biphenyls - PCB 1016 - PCB 1221 - PCB 1232 - PCB-1242 - PCB-1248 - PCB-1254 - PCB-1260	1) Liquid-Liquid Extraction, Gas Chromatographic Method ^[4] 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
97	Pentachlorophenol	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
98	pH	Electrometric Method ^[4]
99	Phenanthrene	1) Liquid-Liquid Extraction, Gas Chromatographic Method ^[4] 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
100	Phenol	1) Distillation, Chloroform Extraction Method ^[4] 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
101	Pyrene	1) Liquid-Liquid Extraction, Gas Chromatographic Method ^[4] 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
102	Selenium	1) Digestion, Hydride Generation/Atomic Absorption Spectrometric Method ^[4] 2) Digestion, Inductively Coupled Plasma Method ^[4]
103	Silver	Digestion, Inductively Coupled Plasma Method ^[4]
104	Styrene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ^[4]
105	1,1,2,2-Tetrachloroethane	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ^[4]
106	Tetrachloroethylene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ^[4]
107	Toluene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ^[4]

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
108	Toxaphene	1) Liquid-Liquid Extraction, Gas Chromatographic Method ^[4] 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
109	TPH (C ₅ - C ₈)	1) Purge and Trap, Gas Chromatographic Method ^[11,21] 2) Purge and Trap, Gas Chromatographic/Mass spectrometric Method ^[11,25]
110	TPH (C ₉ - C ₁₆)	Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method ^[9,21]
111	TPH (C ₁₆ - C ₃₅)	Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method ^[9,21]
112	1,2,4-Trichlorobenzene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ^[4]
113	1,1,1-Trichloroethane	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ^[4]
114	1,1,2-Trichloroethane	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ^[4]
115	Trichloroethylene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ^[4]
116	2,4,5-Trichlorophenol	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
117	2,4,6-Trichlorophenol	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
118	1,3,5-Trimethylbenzene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ^[4]
119	Vanadium	Digestion, Inductively Coupled Plasma Method ^[4]
120	Vinyl acetate	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ^[9]
121	Vinyl chloride	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ^[4]
122	m-Xylene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ^[9]
123	o-Xylene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ^[9]

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
124	p-Xylene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ^[4]
125	Xylene (Total)	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ^[4]
126	Zinc	1) Digestion, Direct Air-Acetylene Flame Method ^[4] 2) Digestion, Electrothermal Atomic Absorption Spectrometric Method ^[4] 3) Digestion, Inductively Coupled Plasma Method ^[4]

อากาศเสีย (ปล่อยระบาย) จำนวน 25 รายการ

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
1	Antimony	Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method ^[5]
2	Arsenic	1) Isokinetic Sampling, Digestion, Hydride Generation/Atomic Absorption Spectrometric Method ^[5] 2) Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method ^[5]
3	Cadmium	1) Isokinetic Sampling, Digestion, Direct Air-Acetylene Flame Method ^[5] 2) Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method ^[5]
4	Carbon Monoxide	Instrumental Analyzer Method ^[5]
5	Chlorine	Isokinetic Sampling, Ion Chromatographic Method ^[5]
6	Chromium	1) Isokinetic Sampling, Digestion, Direct Air-Acetylene Flame Method ^[5] 2) Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method ^[5]
7	Cobalt	Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method ^[5]
8	Copper	1) Isokinetic Sampling, Digestion, Direct Air-Acetylene Flame Method ^[5] 2) Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method ^[5]
9	Cresol	Absorption Sampling, Gas Chromatographic Method ^[5]

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
10	Dioxins/Furans	Isokinetic Sampling ⁽⁵⁾
11	Hydrogen Chloride	Isokinetic Sampling, Ion Chromatographic Method ⁽⁵⁾
12	Hydrogen Fluoride	Isokinetic Sampling, Ion Chromatographic Method ⁽⁵⁾
13	Hydrogen Sulfide	Absorption Sampling, Iodometric Method ⁽⁵⁾
14	Lead	1) Isokinetic Sampling, Digestion, Direct Air-Acetylene Flame Method ⁽⁵⁾ 2) Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method ⁽⁵⁾
15	Manganese	1) Isokinetic Sampling, Digestion, Direct Air-Acetylene Flame Method ⁽⁵⁾ 2) Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method ⁽⁵⁾
16	Mercury	Isokinetic Sampling, Digestion, Cold-Vapor Atomic Absorption Spectrometric Method ⁽⁵⁾
17	Nickel	1) Isokinetic Sampling, Digestion, Direct Air-Acetylene Flame Method ⁽⁵⁾ 2) Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method ⁽⁵⁾
18	Opacity	Ringelmann's Method ⁽¹⁾
19	Oxides of Nitrogen	1) Absorption Sampling, Phenoldisulfonic acid Method ⁽⁵⁾ 2) Instrumental Analyzer Method ⁽⁵⁾
20	Selenium	1) Isokinetic Sampling, Digestion, Hydride Generation/Atomic Absorption Spectrometric Method ⁽⁵⁾ 2) Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method ⁽⁵⁾
21	Sulfur Dioxide	1) Absorption Sampling, Barium-Thorin Titrimetric Method ⁽⁵⁾ 2) Instrumental Analyzer Method ⁽⁵⁾
22	Sulfuric Acid	Isokinetic Sampling, Barium-Thorin Titrimetric Method ⁽⁵⁾
23	Total Suspended Particulate	Isokinetic Sampling, Gravimetric Method ⁽⁵⁾
24	Vanadium	Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method ⁽⁵⁾
25	Xylene	1) Bag Sampling, Gas Chromatographic Method ⁽⁵⁾ 2) Adsorption Sampling, Gas Chromatographic Method ⁽⁵⁾

สิ่งปฏิกูลหรือวัสดุที่ไม่ใช้แล้ว จำนวน 35 รายการ

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
1	Aldrin	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method ^[2,9,22] 2) Ultrasonic Extraction, Gas Chromatographic Method ^[10,22]
2	Antimony	Digestion, Inductively Coupled Plasma Method ^[7,13]
3	Arsenic	1) Waste Extraction, Digestion, Hydride Generation/Atomic Absorption Spectrometric Method ^[2,6,15] 2) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[2,6,13] 3) Digestion, Hydride Generation/Atomic Absorption Spectrometric Method ^[7,15] 4) Digestion, Inductively Coupled Plasma Method ^[7,13]
4	Barium	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[2,6,13] 2) Digestion, Inductively Coupled Plasma Method ^[7,13]
5	Beryllium	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[2,6,13] 2) Digestion, Inductively Coupled Plasma Method ^[7,13]
6	Cadmium	1) Waste Extraction, Digestion, Flame Atomic Absorption Spectrometric Method ^[2,6,14] 2) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[2,6,13] 3) Digestion, Flame Atomic Absorption Spectrometric Method ^[7,14] 4) Digestion, Inductively Coupled Plasma Method ^[7,13]
7	Chlordane	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method ^[2,9,22] 2) Ultrasonic Extraction, Gas Chromatographic Method ^[10,22]
8	Chromium	1) Waste Extraction, Digestion, Flame Atomic Absorption Spectrometric Method ^[2,6,14] 2) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[2,6,13]

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
9	Chromium (III)	<p>3) Digestion, Flame Atomic Absorption Spectrometric Method^[7,14]</p> <p>4) Digestion, inductively Coupled Plasma Method^[7,13]</p> <p>1) Waste Extraction, Digestion, Flame Atomic Absorption Spectrometric Method; Waste Extraction, Colorimetric Method; Calculation^[2,6,14,16]</p> <p>2) Waste Extraction, Digestion, Inductively Coupled Plasma Method; Waste Extraction, Colorimetric Method; Calculation^[2,6,13,16]</p> <p>3) Digestion, Flame Atomic Absorption Spectrometric Method; Alkaline Digestion, Colorimetric Method; Calculation^[7,8,14,16]</p> <p>4) Digestion, Inductively Coupled Plasma Method; Alkaline Digestion, Colorimetric Method; Calculation^[7,8,13,16]</p>
10	Chromium (VI)	<p>1) Waste Extraction, Colorimetric Method^[2,16]</p> <p>2) Alkaline Digestion, Colorimetric Method^[6,16]</p>
11	Cobalt	<p>1) Waste Extraction, Digestion, Inductively Coupled Plasma Method^[7,6,13]</p> <p>2) Digestion, Inductively Coupled Plasma Method^[7,13]</p>
12	Copper	<p>1) Waste Extraction, Digestion, Flame Atomic Absorption Spectrometric Method^[2,6,14]</p> <p>2) Waste Extraction, Digestion, Inductively Coupled Plasma Method^[2,6,13]</p> <p>3) Digestion, Flame Atomic Absorption Spectrometric Method^[7,14]</p> <p>4) Digestion, Inductively Coupled Plasma Method^[7,13]</p>
13	2,4-D	<p>1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method^[7,9,77]</p> <p>2) Ultrasonic Extraction, Gas Chromatographic Method^[10,22]</p>
14	DDD	<p>1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method^[7,9,77]</p> <p>2) Ultrasonic Extraction, Gas Chromatographic Method^[10,22]</p>

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
15	DDE	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method ^[2,9,22] 2) Ultrasonic Extraction, Gas Chromatographic Method ^[10,22]
16	DDT	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method ^[2,9,22] 2) Ultrasonic Extraction, Gas Chromatographic Method ^[10,22]
17	Dieldrin	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method ^[2,9,22] 2) Ultrasonic Extraction, Gas Chromatographic Method ^[10,22]
18	Endrin	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method ^[2,9,22] 2) Ultrasonic Extraction, Gas Chromatographic Method ^[10,22]
19	Heptachlor	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method ^[2,9,22] 2) Ultrasonic Extraction, Gas Chromatographic Method ^[10,22]
20	Lead	1) Waste Extraction, Digestion, Flame Atomic Absorption Spectrometric Method ^[2,6,14] 2) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[2,6,13] 3) Digestion, Flame Atomic Absorption Spectrometric Method ^[7,14] 4) Digestion, Inductively Coupled Plasma Method ^[7,13]
21	Lindane	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method ^[2,9,22] 2) Ultrasonic Extraction, Gas Chromatographic Method ^[10,22]
22	Mercury	1) Waste Extraction, Digestion, Cold-Vapor Atomic Absorption Spectrometric Method ^[2,17] 2) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[2,6,13]

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
23	Methoxychlor	3) Digestion, Cold-Vapor Atomic Absorption Spectrometric Method ^[18] 4) Digestion, Inductively Coupled Plasma Method ^[7,13] 5) Thermal Decomposition Amalgamation and Atomic Absorption Spectrometric Method ^[19] 1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method ^[2,9,22] 2) Ultrasonic Extraction, Gas Chromatographic Method ^[10,22]
24	Molybdenum	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[2,6,13] 2) Digestion, Inductively Coupled Plasma Method ^[7,13]
25	Nickel	1) Waste Extraction, Digestion, Flame Atomic Absorption Spectrometric Method ^[2,6,14] 2) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[2,6,15] 3) Digestion, Flame Atomic Absorption Spectrometric Method ^[7,14] 4) Digestion, Inductively Coupled Plasma Method ^[7,13]
26	Polychlorinated Biphenyls - Aroclor 1016 - Aroclor 1221 - Aroclor 1232 - Aroclor 1242 - Aroclor 1248 - Aroclor 1254 - Aroclor 1260 - 2-Chlorobiphenyl - 2,3-Dichlorobiphenyl - 2,2',5-Trichlorobiphenyl - 2,4',5-Trichlorobiphenyl - 2,2',3,5'-Tetrachlorobiphenyl - 2,2',5,5'-Tetrachlorobiphenyl - 2,3',4,4'-Tetrachlorobiphenyl - 2,2',3,4,5'-Pentachlorobiphenyl	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method ^[2,9,23] 2) Ultrasonic Extraction, Gas Chromatographic Method ^[10,23]

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
	- 2,2',4,5,5'- Pentachlorobiphenyl - 2,3,3',4',6- Pentachlorobiphenyl - 2,2',3,4,4',5'- Hexachlorobiphenyl - 2,2',3,4,5,5'- Hexachlorobiphenyl - 2,2',3,5,5',6- Hexachlorobiphenyl - 2,2',4,4',5,5'- Hexachlorobiphenyl - 2,2',3,3',4,4',5- Heptachlorobiphenyl - 2,2',3,4,4',5,5'- Heptachlorobiphenyl - 2,2',3,4,4',5',6- Heptachlorobiphenyl - 2,2',3,4',5,5',6- Heptachlorobiphenyl - 2,2',3,3',4,4',5,5',6- Nonachlorobiphenyl 27 Pentachlorophenol	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[2,9,28] 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[10,26] Electrometric Method ^[31,32] 28 pH 29 Selenium 1) Waste Extraction, Digestion, Hydride Generation/Atomic Absorption Spectrometric Method ^[2,6,20] 2) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[2,6,13] 3) Digestion, Hydride Generation/Atomic Absorption Spectrometric Method ^[7,20] 4) Digestion, Inductively Coupled Plasma Method ^[7,13]

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
30	Silver	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[2,6,13]
31	Thallium	2) Digestion, Inductively Coupled Plasma Method ^[7,13] 1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[2,6,13]
32	Toxaphene	2) Digestion, Inductively Coupled Plasma Method ^[7,13] 1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method ^[2,9,22]
33	Trichloroethylene	2) Ultrasonic Extraction, Gas Chromatographic Method ^[10,22] 1) Waste Extraction, Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[2,12,25]
34	Vanadium	2) Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[12,25] 1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[2,6,13]
35	Zinc	2) Digestion, Inductively Coupled Plasma Method ^[7,13] 1) Waste Extraction, Digestion, Flame Atomic Absorption Spectrometric Method ^[2,6,14] 2) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[2,6,13] 3) Digestion, Flame Atomic Absorption Spectrometric Method ^[7,14] 4) Digestion, Inductively Coupled Plasma Method ^[7,13]

ดิน จำนวน 125 รายการ

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
1	Acenaphthene	1) Ultrasonic Extraction, Gas Chromatographic Method ^[10,24] 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[10,26]
2	Acetone	Purge and Trap, Gas Chromatographic Spectrometric Method ^[2,22]

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
3	Aldrin	1) Ultrasonic Extraction, Gas Chromatographic Method ^[10,22] 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[10,26]
4	Anthracene	1) Ultrasonic Extraction, Gas Chromatographic Method ^[10,26] 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[10,26]
5	Antimony	Digestion, Inductively Coupled Plasma Method ^[7,13]
6	Arsenic	1) Digestion, Hydride Generation/Atomic Absorption Spectrometric Method ^[7,15] 2) Digestion, Inductively Coupled Plasma Method ^[7,13]
7	Atrazine	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[10,26]
8	Barium	Digestion, Inductively Coupled Plasma Method ^[7,13]
9	Benz(a)anthracene	1) Ultrasonic Extraction, Gas Chromatographic Method ^[10,26] 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[10,26]
10	Benzene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[12,25]
11	Benzo(b)fluoranthene	1) Ultrasonic Extraction, Gas Chromatographic Method ^[10,24] 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[10,26]
12	Benzo(k)fluoranthene	1) Ultrasonic Extraction, Gas Chromatographic Method ^[10,24] 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[10,26]
13	Benzoic acid	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[10,26]
14	Benzo(a)pyrene	1) Ultrasonic Extraction, Gas Chromatographic Method ^[10,24] 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[10,26]

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
15	Benzo(g,h,i)perylene	1) Ultrasonic Extraction, Gas Chromatographic Method ^[10,22] 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[10,26]
16	Beryllium	Digestion, Inductively Coupled Plasma Method ^[7,13]
17	Bis(2-chloroethyl)ether	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[10,26]
18	Bis(2-ethylhexyl)phthalate	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[10,26]
19	Bromodichloromethane	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[12,25]
20	Bromoform	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[12,25]
21	Butanol	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[12,25]
22	Butyl benzyl phthalate	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[10,26]
23	Cadmium	1) Digestion, Flame Atomic Absorption Spectrometric Method ^[7,14] 2) Digestion, Inductively Coupled Plasma Method ^[7,13]
24	Carbazole	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[10,26]
25	Carbon disulfide	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[12,25]
26	Carbon tetrachloride	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[12,25]
27	Chlordane	1) Ultrasonic Extraction, Gas Chromatographic Method ^[10,22] 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[10,26]
28	p-Chloroaniline	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[10,26]
29	Chlorobenzene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[12,25]
30	Chlorodibromomethane	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[12,25]

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
31	Chloroform	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[12,25]
32	2-Chlorophenol	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[13,26]
33	Chromium	1) Digestion, Flame Atomic Absorption Spectrometric Method ^[7,14] 2) Digestion, Inductively Coupled Plasma Method ^[7,13]
34	Chromium (III)	1) Digestion, Flame Atomic Absorption Spectrometric Method; Alkaline Digestion, Colorimetric Method; Calculation ^[7,8,14,16] 2) Digestion, Inductively Coupled Plasma Method; Alkaline Digestion, Colorimetric Method; Calculation ^[7,8,13,16]
35	Chromium (VI)	Alkaline Digestion, Colorimetric Method ^[8,16]
36	Chrysene	1) Ultrasonic Extraction, Gas Chromatographic Method ^[10,24] 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[10,26]
37	Cyanide	Extraction, Distillation, Colorimetric Method ^[26,29,30]
38	2,4-D	Ultrasonic Extraction, Gas Chromatographic Method ^[27]
39	DDD	1) Ultrasonic Extraction, Gas Chromatographic Method ^[10,22] 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[10,26]
40	DDE	1) Ultrasonic Extraction, Gas Chromatographic Method ^[10,22] 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[10,26]
41	DDT	1) Ultrasonic Extraction, Gas Chromatographic Method ^[10,22] 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[10,26]
42	Dibenz(a,h)anthracene	1) Ultrasonic Extraction, Gas Chromatographic Method ^[10,24] 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[10,26]

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
43	Di-n-butyl phthalate	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^(10,26)
44	1,2-Dichlorobenzene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^(12,25)
45	1,3-Dichlorobenzene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^(12,25)
46	1,4-Dichlorobenzene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^(12,25)
47	3,3'-Dichlorobenzidine	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^(10,25)
48	1,1-Dichloroethane	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^(12,25)
49	1,2-Dichloroethane	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^(12,25)
50	1,1-Dichloroethylene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^(12,25)
51	cis-1,2-Dichloroethylene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^(12,25)
52	trans-1,2-Dichloroethylene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^(12,25)
53	2,4-Dichlorophenol	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^(10,26)
54	1,2-Dichloropropane	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^(12,25)
55	1,3-Dichloropropane	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^(12,25)
56	1,3-Dichloropropene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^(12,25)
57	Dieldrin	1) Ultrasonic Extraction, Gas Chromatographic Method ^(10,22) 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^(10,25)
58	Diethyl phthalate	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^(10,26)
59	2,4-Dimethylphenol	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^(10,26)

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
60	2,4-Dinitrophenol	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[10,26]
61	2,4-Dinitrotoluene	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[10,26]
62	2,6-Dinitrotoluene	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[10,26]
63	Di-n-Octyl phthalate	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[10,26]
64	Endosulfan	1) Ultrasonic Extraction, Gas Chromatographic Method ^[10,22] 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[10,26]
65	Endrin	1) Ultrasonic Extraction, Gas Chromatographic Method ^[10,22] 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[10,26]
66	Ethylbenzene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[12,25]
67	Fluoranthene	1) Ultrasonic Extraction, Gas Chromatographic Method ^[10,24] 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[10,26]
68	Fluorene	1) Ultrasonic Extraction, Gas Chromatographic Method ^[10,24] 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[10,26]
69	Heptachlor	1) Ultrasonic Extraction, Gas Chromatographic Method ^[10,22] 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[10,26]
70	Heptachlor epoxide	1) Ultrasonic Extraction, Gas Chromatographic Method ^[10,22] 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[10,26]

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
71	Hexachlorobenzene	1) Ultrasonic Extraction, Gas Chromatographic Method ^[10,22] 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[10,25]
72	Hexachloro-1,3-butadiene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[1,2,25]
73	n-Hexane	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[12,25]
74	α -HCH	1) Ultrasonic Extraction, Gas Chromatographic Method ^[10,22] 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[10,26]
75	β -HCH	1) Ultrasonic Extraction, Gas Chromatographic Method ^[10,22] 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[10,26]
76	γ -HCH	1) Ultrasonic Extraction, Gas Chromatographic Method ^[10,22] 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[10,26]
77	Hexachlorocyclopentadiene	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[10,26]
78	Hexachloroethane	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[10,26]
79	indeno(1,2,3-cd)pyrene	1) Ultrasonic Extraction, Gas Chromatographic Method ^[10,26] 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[10,26]
80	Isophorone	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[10,26]
81	Lead	1) Digestion, Flame Atomic Absorption Spectrometric Method ^[7,14] 2) Digestion, Inductively Coupled Plasma Atomic Absorption Spectrometric Method ^[7,14]
82	Manganese	1) Digestion, Flame Atomic Absorption Spectrometric Method ^[7,14] 2) Digestion, Inductively Coupled Plasma Method ^[7,13]

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
83	Mercury	1) Digestion, Cold-Vapor Atomic Absorption Spectrometric Method ^[18] 2) Digestion, Inductively Coupled Plasma Method ^[7,15] 3) Thermal Decomposition Amalgamation and Atomic Absorption Spectrometric Method ^[19]
84	Methanol	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[12,25]
85	Methoxychlor	1) Ultrasonic Extraction, Gas Chromatographic Method ^[10,22] 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[10,26]
86	Methyl bromide	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[12,25]
87	Methylene chloride	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[12,25]
88	2-Methylphenol	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[10,26]
89	2-Methylnaphthalene	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[10,26]
90	Methyl tert-butyl ether	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[12,25]
91	Naphthalene	1) Ultrasonic Extraction, Gas Chromatographic Method ^[10,24] 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[10,26]
92	Nickel	1) Digestion, Flame Atomic Absorption Spectrometric Method ^[7,14] 2) Digestion, Inductively Coupled Plasma Method ^[7,13]
93	Nitrobenzene	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[10,26]
94	N-Nitrosodiphenylamine	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[10,26]
95	N-Nitrosodi-n-propylamine	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[10,26]

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
96	<p>Polychlorinated Biphenyls</p> <ul style="list-style-type: none"> - Aroclor 1016 - Aroclor 1221 - Aroclor 1232 - Aroclor 1242 - Aroclor 1248 - Aroclor 1254 - Aroclor 1260 <p>Polychlorinated Biphenyls</p> <ul style="list-style-type: none"> - 2-Chlorobiphenyl - 2,3-Dichlorobiphenyl - 2,2',5-Trichlorobiphenyl - 2,4',5-Trichlorobiphenyl - 2,2',3,5'-Tetrachlorobiphenyl - 2,2',5,5'-Tetrachlorobiphenyl - 2,3',4,4'-Tetrachlorobiphenyl - 2,2',3,4,5'- <p>Pentachlorobiphenyl</p> <ul style="list-style-type: none"> - 2,2',4,5,5'- <p>Pentachlorobiphenyl</p> <ul style="list-style-type: none"> - 2,3,3',4',5'- <p>Pentachlorobiphenyl</p> <ul style="list-style-type: none"> - 2,2',3,4,4',5'- <p>Hexachlorobiphenyl</p> <ul style="list-style-type: none"> - 2,2',3,4,5,5'- <p>Hexachlorobiphenyl</p> <ul style="list-style-type: none"> - 2,2',3,5,5',6- <p>Hexachlorobiphenyl</p> <ul style="list-style-type: none"> - 2,2',4,4',5,5'- <p>Hexachlorobiphenyl</p> <ul style="list-style-type: none"> - 2,2',3,3',4,4',5- <p>Heptachlorobiphenyl</p> <ul style="list-style-type: none"> - 2,2',3,4,4',5,5'- <p>Heptachlorobiphenyl</p> <ul style="list-style-type: none"> - 2,2',3,4,4',5',6- <p>Heptachlorobiphenyl</p>	<p>1) Ultrasonic Extraction, Gas Chromatographic Method^(10,23)</p> <p>2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method^(10,26)</p> <p>Ultrasonic Extraction, Gas Chromatographic Me</p>

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
97	- 2,2',3,4',5,5',6- Heptachlorobiphenyl	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[10,26]
98	- 2,2',3,3',4,4',5,5',6- Nonachlorobiphenyl	1) Ultrasonic Extraction, Gas Chromatographic Method ^[10,24] 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[10,26]
99	Pentachlorophenol	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[10,26]
100	Phenanthrene	1) Ultrasonic Extraction, Gas Chromatographic Method ^[10,24] 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[10,26]
101	Pyrene	1) Digestion, Hydride Generation/Atomic Absorption Spectrometric Method ^[7,22] 2) Digestion, Inductively Coupled Plasma Method ^[7,13]
102	Selenium	Digestion, Inductively Coupled Plasma Method ^[7,13]
103	Silver	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[12,25]
104	Styrene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[12,25]
105	1,1,2,2-Tetrachloroethane	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[12,25]
106	Tetrachloroethylene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[12,25]
107	Toluene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[12,25]
108	Toxaphene	Ultrasonic Extraction, Gas Chromatographic Method ^[10,22]
109	TPH (C ₅ -C ₈)	1) Purge and Trap, Gas Chromatographic Method ^[12,21] 2) Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[12,25]
110	TPH (C ₈ -C ₁₆)	Ultrasonic Extraction, Gas Chromatographic Method ^[10,22]
111	TPH (C ₁₆ -C ₃₅)	Ultrasonic Extraction, Gas Chromatographic Method ^[10,21]
112	1,2,4-Trichlorobenzene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[12,25]

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
112	1,1,1-Trichloroethane	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^(12,25)
113	1,1,2-Trichloroethane	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^(12,25)
114	Trichloroethylene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^(12,25)
115	2,4,5-Trichlorophenol	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^(10,26)
116	2,4,6-Trichlorophenol	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^(10,26)
117	1,3,5-Trimethylbenzene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^(12,25)
118	Vanadium	Digestion, Inductively Coupled Plasma Method ^(7,13)
119	Vinyl acetate	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^(12,25)
120	Vinyl chloride	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^(12,25)
121	m-Xylene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^(12,25)
122	o-Xylene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^(12,25)
123	p-Xylene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^(12,25)
124	Xylene (Total)	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^(12,25)
125	Zinc	1) Digestion, Flame Atomic Absorption Spectrometric Method ^(7,14) 2) Digestion, Inductively Coupled Plasma Method ^(7,13)

เอกสารอ้างอิง

- กระทรวงอุตสาหกรรม. ประกาศกระทรวงอุตสาหกรรม, พ.ศ. 2549. เรื่อง กำหนดค่าปริมาณเข้มข้นควันที่เจือปนในอากาศที่ระบายออกจากปล่องของหม้อน้ำโรงสีข้าวที่ใช้ถ่านหินเป็นเชื้อเพลิง. ราชกิจจานุเบกษา. 4 ธันวาคม 2549. เล่มที่ 123 ตอนพิเศษ 125 ง
- กระทรวงอุตสาหกรรม. ประกาศกระทรวงอุตสาหกรรม, พ.ศ. 2553. เรื่อง การกำจัดสิ่งปฏิกูลหรือวัสดุที่ไม่ใช้แล้ว. ราชกิจจานุเบกษา. 25 มกราคม 2549. เล่มที่ 123 ตอนพิเศษ 11 ง

3. สมาคมวิศวกรรมสิ่งแวดล้อมแห่งประเทศไทย. คู่มือวิเคราะห์น้ำเสีย. พิมพ์ครั้งที่ 4. กรุงเทพฯ: เรือนแก้วการพิมพ์, 2547.
4. APHA, AWWA, WEF. **Standard Methods for the Examination of Water and Wastewater**. 23rd ed. Washington, DC: APHA, 2017.
5. United States Environmental Protection Agency. **Standards of Performance for New Stationary Sources**. 40 C-FR 60. Appendix A, 2019.
6. United States Environmental Protection Agency. **Test Methods for Evaluation Solid Waste Physical/Chemical Methods**. SW-846, 1997.
7. United States Environmental Protection Agency. **Test Methods for Evaluation Solid Waste Physical/Chemical Methods. Acid Digestion of Sediments, Sludges, and Soils**. SW-846 Method 3050B, 1996.
8. United States Environmental Protection Agency. **Test Methods for Evaluation Solid Waste Physical/Chemical Methods. Alkaline Digestion for Hexavalent Chromium**. SW-846 Method 3060A, 1996.
9. United States Environmental Protection Agency. **Test Methods for Evaluation Solid Waste 3. Physical/Chemical Methods. Separatory Funnel Liquid-Liquid Extraction**. SW-846 Method 3510C, 1996.
10. United States Environmental Protection Agency. **Test Methods for Evaluation Solid Waste Physical/Chemical Methods. Ultrasonic Extraction**. SW-846 Method 3550C, 2007.
11. United States Environmental Protection Agency. **Test Methods for Evaluation Solid Waste Physical/Chemical Methods. Purge and Trap for Aqueous Samples**. SW-846 Method 5030C, 2003.
12. United States Environmental Protection Agency. **Test Methods for Evaluation Solid Waste Physical/Chemical Methods. Closed System Purge and Trap and Extraction for Volatile Organics in Soil and Waste Sample**. SW-846 Method 5035A, 2000.
13. United States Environmental Protection Agency. **Test Methods for Evaluation Solid Waste Physical/Chemical Methods. Inductively Coupled Plasma-Optical Emission Spectrometry**. SW-846 Method 6010D, 2014.
14. United States Environmental Protection Agency. **Test Methods for Evaluation Solid Waste Physical/Chemical Methods. Flame Atomic Absorption Spectrophotometry**. SW-846 Method 7000B, 2007.
15. United States Environmental Protection Agency. **Test Methods for Evaluation Solid Waste Physical/Chemical Methods. Arsenic (Atomic Absorption, Gaseous Method)**. SW-846 Method 7061A, 1992.

16. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Chromium, Hexavalent (Colorimetric)**. SW-846 Method 7196A, 1992.

17. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Mercury in Liquid Waste (Manual Cold Vapor Technique)**. SW-846 Method 7470A, 1994.

18. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Mercury in Solid or Semisolid Waste (Manual Cold-Vapor Technique)**. SW-846 Method 7471B, 1998.

19. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Mercury in Solids and Solutions by Thermal Decomposition, Amalgamation, and Atomic Absorption Spectrophotometry**. SW-846 Method 7473, 2007.

20. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Selenium (Atomic Absorption, Borohydride Reduction)**. SW-846 Method 7742, 1994.

21. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Nonhalogenated Organics Using GC/FID**. SW-846 Method 8015D, 2003.

22. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Organochlorine Pesticides by Gas Chromatography**. SW-846 Method 8081B, 2007.

23. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Polychlorinated Biphenyls (PCBs) by Gas Chromatography**. SW-846 Method 8082A, 2007.

24. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Polynuclear Aromatic Hydrocarbons**. SW-846 Method 8100, 1980.

25. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Volatile Organic Compounds by Gas Chromatography/Mass Spectrometry**. SW-846 Method 8260D, 2018.

26. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Semivolatile Organic Compounds by Gas Chromatography/Mass Spectrometry**. SW-846 Method 8270E, 2018.

27. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Chlorinated Herbicides by GC Using Methylation or Pentafluorobenzoylation Derivatization**. SW-846 Method 8151A, 1996.

28. United States...

28. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Total and Amenable Cyanide : Distillation. SW-846 Method 9010C**, 2004.

29. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Cyanide Extraction Procedure for Solids and Oils. SW-846 Method 9013A**, 2014.

30. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Cyanide in Waters and Extracts using Titrimetric and Manual Spectrophotometric Procedures. SW-846 Method 9014**, 2014.

31. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **pH Electrometric Measurement. SW-846 Method 9040C**, 2004.

32. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Soil and Waste pH. SW-846 Method 9045D**, 2004



ดำเนินการโดย