

สำเนาเอกสารสอบเทียบเครื่องมือวัด

Mettler-Toledo (Thailand) Ltd.
846/4 - 846/5 Lasaile Rd., Bangna Tai Sub-District
Bangna District, Bangkok 10260
+66 2723 0382
MT-TH.ServiceSupport@mt.com



MSC-TIS-TIS 17025
CALIBRATION 0062

Accuracy Calibration Certificate

Customer

Company: EASTERN THAI CONSULTING 1992 CO., LTD.
Address: 683 Moo 11, Sukhaphiban 8 Rd., Nong Kham
City: Sriracha
Zip / Postal: 20230
State / Province: Chonburi
Order Number: 033280040
Contact: Sasiporn N.

Weighing Device

Manufacturer: Mettler Toledo
Model: MS204TS/00
Serial No.: B904136539
Building: Laboratory
Floor: 1
Room: Balance
Instrument Type: Weighing Instrument
Asset Number: LABE 05/4
Terminal Model: N/A
Terminal Serial No.: N/A
Terminal Asset No.: N/A

Range	Max. Capacity	Readability (d)
1	220 g	0.0001 g

Procedure

Calibration Guideline:
METTLER TOLEDO Work Instruction:
EURAMET cg-18 v. 4.0 (11/2015)
CP/W002/20

This calibration certificate contains measurements for As Found and As Left calibrations.
The sensitivity/span of the weighing instrument was adjusted before As Found and As Left calibrations with a built-in weight.
In accordance with EURAMET cg-18 (11/2015), the test loads were selected to reflect the specific use of the weighing device or to accommodate specific calibration conditions.

	Temperature		Humidity	
As Found	Start: 23.4 °C	End: 23.4 °C	Start: 50.6 %	End: 50.6 %
As Left	Start: 23.8 °C	End: 23.4 °C	Start: 51.8 %	End: 51.2 %

As Found Calibration Date: 05-Feb-2024
As Left Calibration Date: 05-Feb-2024
Issue Date: 05-Feb-2024
Calibrator: Sathaporn T
Sathaporn Tabson

Approved Signatory:

Sathaporn T

Technical Manager / Head of Calibration Center

COPY

Measurement Results

Repeatability


Test Load: 100 g		As Found	As Left
1	99.9996 g	100.0001 g	As Found
2	99.9997 g	100.0001 g	As Left
3	99.9997 g	100.0000 g	As Found
4	99.9996 g	100.0001 g	As Left
5	99.9997 g	100.0001 g	As Found
6	99.9996 g	100.0000 g	As Left
7	99.9997 g	100.0001 g	As Found
8	99.9996 g	100.0000 g	As Left
9	99.9996 g	100.0001 g	As Found
10	99.9996 g	100.0001 g	As Left
Standard Deviation		0.00005 g	

1 (Found Point)
256
4d
3d
2d
1d

The "d" in the graph represents the readability of the range interval in which the test was performed.
The results of this graph are based upon the absolute values of the differences from the mean value.

Eccentricity

Test Load: 100 g		As Found	As Left
1	99.9996 g	100.0000 g	As Found
2	99.9996 g	100.0000 g	As Left
3	99.9997 g	100.0001 g	As Found
4	99.9996 g	100.0001 g	As Left
5	99.9996 g	100.0000 g	As Found
Maximum Deviation		0.0001 g	

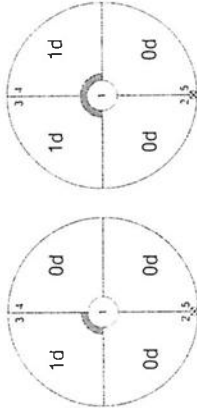

The "d" in the graph represents the readability of the range interval in which the test was performed.

Error of Indication

As Found	Reference Value	Indication	Error of Indication	Expanded Uncertainty	k
1	0.0000 g	0.0000 g	0.0000 g	0.12 mg	2
2	0.0100 g	0.0100 g	0.0000 g	0.13 mg	2
3	0.0500 g	0.0499 g	-0.0001 g	0.13 mg	2
4	0.1000 g	0.0998 g	-0.0001 g	0.13 mg	2
5	1.0000 g	0.9999 g	-0.0001 g	0.13 mg	2
6	5.0000 g	4.9999 g	-0.0001 g	0.14 mg	2
7	10.0000 g	9.9999 g	-0.0001 g	0.14 mg	2
8	50.0000 g	49.9997 g	-0.0003 g	0.16 mg	2
9	100.0000 g	99.9995 g	-0.0005 g	0.20 mg	2
10 ¹	149.9999 g	149.9993 g	-0.0006 g	0.31 mg	2
11 ¹	199.9998 g	199.9990 g	-0.0008 g	0.35 mg	2

As Left

Reference Value	Indication	Error of Indication	Expanded Uncertainty	k
1	0.0000 g	0.0000 g	0.11 mg	2
2	0.0100 g	0.0000 g	0.13 mg	2
3	0.0500 g	0.0000 g	0.13 mg	2
4	0.1000 g	0.0000 g	0.13 mg	2
5	1.0000 g	0.0001 g	0.13 mg	2
6	5.0000 g	0.0000 g	0.13 mg	2
7	10.0000 g	0.0001 g	0.14 mg	2
8	50.0000 g	0.0001 g	0.15 mg	2
9 ¹	100.0000 g	0.0001 g	0.20 mg	2
10 ¹	149.9999 g	0.0001 g	0.31 mg	2
11 ¹	199.9998 g	0.0001 g	0.35 mg	2

¹The calculated uncertainty was replaced by the CMC (Calibration and Measurement Capabilities) value because the calculated uncertainty was smaller than the CMC value.

As Found

◆ As Left



For improved legibility of the graphics only increasing measurement points are shown and measurement points close to zero are not displayed.

Calibration Points [g]

The uncertainty stated is the expanded uncertainty at calibration obtained by multiplying the standard combined uncertainty by the coverage factor k – which can be larger than 2 according to EURAMET cg-18. The value of the measurand lies within the assigned range of values with a probability of approximately 95%.

The results of this calibration certificate relate only to the calibrated item.

Test Equipment

All weights used for metrological testing are traceable to national or international standards. The weights were calibrated and certified by an accredited calibration laboratory.

Weight Set 1: OIML E2

Weight Set No.: WS32
Certificate Number: 188109
Date of Issue: 25-Sep-2023
Calibration Due Date: 25-Mar-2025

Weight Set 2: OIML E2

Weight Set No.: WS85
Certificate Number: 188113
Date of Issue: 27-Sep-2023
Calibration Due Date: 26-Mar-2025

Thermo Baro Hygrometer

Equipment No.: IN74
Certificate Number: SG-H-00418/66
Date of Issue: 19-May-2023
Calibration Due Date: 18-May-2024

Remarks

FACT adjustment functionality activated
Equipment condition: Good
Next calibration according to customer's procedure
Calibration data not decide by calibration laboratory

End of Accredited Section

The information below and any attachments to this calibration certificate are not part of the accredited calibration.

Measurement Uncertainty of the Weighing Instrument in Use

Stated is the expanded uncertainty with $k=2$ in use. The formula shall be used for the estimation of the uncertainty under consideration of the errors of indication. The value R represents the net load indication in the unit of measure of the device.

Temperature coefficient for the evaluation of the measurement uncertainty in use:

 $1.5 \cdot 10^{-6} / \text{K}$

Temperature range on site for the evaluation of the measurement uncertainty in use

5X

Linearization of Uncertainty Equation


Range		As Found	As Left
	d		
1	0.0001 g	220 g	$U_1 = 0.13 \text{ mg} + 0.0101 \text{ mole} \cdot R$ $U_2 = 0.13 \text{ mg} + 0.00616 \text{ mole} \cdot R$

$$U_1 = 0.13 \text{ mg} + 0.0101 \text{ mg/g} \cdot R$$

To optimize the stability of the linearization, besides of the zero load only increasing measurement points with a test load of 5% of the measurement range or larger are taken for the calculation of the linear equation.

Absolute and Relative Measurement Uncertainty In Use for Various Net Indications (Examples)

Net Indication	As Found	As Left
0.0220 g	0.13 mg	0.59%
0.2200 g	0.13 mg	0.060%
2.2000 g	0.15 mg	0.0069%
22.0000 g	0.35 mg	0.0016%
220.0000 g	2.4 mg	0.0011%
		0.00068%

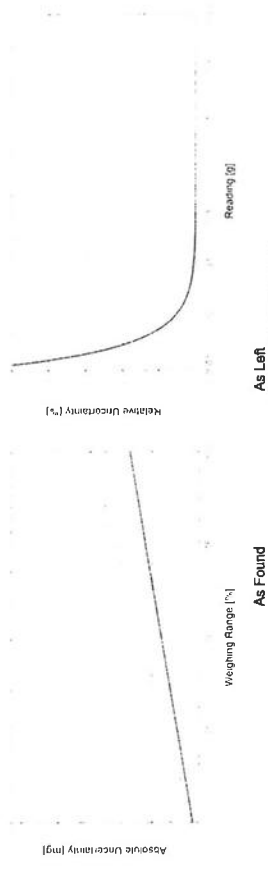

COPIES



**GWP®
Certificate**

Attachment to Calibration Certificate:
TH4004-091-020524-ACC-TH
GWP® Certificate

As Found

As Left

The weighing device meets the given process requirements.

The weighing device meets the given process requirements.

Tests Performed:

As Found

As Left


Process Requirements

Weighing Tolerance: 1%

Smallest Net Weight: 1.0000 g

Safety Factor: 2

Safe Weighing Range

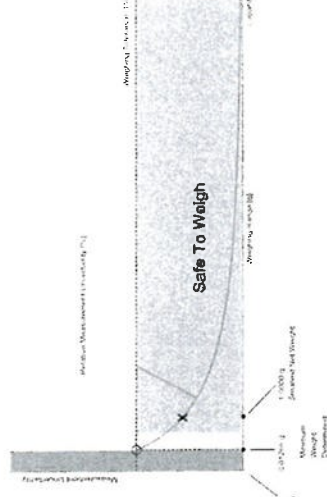

While the values in this graph reflect the actual calibration results, the measurement uncertainty curves are simply a visual representation. This graph reflects As Left testing, unless only As Found was performed.

100

Minimum Weight

As Found Minimum Weight Table

Minimum weights for different weighing tolerances and safety factors					
Tolerance	Safety Factor				
	1	2	3	5	10
0.1%	0.13300 g	0.26873 g	0.40728 g	0.69320 g	1.46405 g
0.2%	0.06616 g	0.13300 g	0.20051 g	0.33764 g	0.69320 g
0.5%	0.02638 g	0.05288 g	0.07947 g	0.13300 g	0.26873 g
1%	0.01318 g	0.02638 g	0.03962 g	0.06616 g	0.13300 g
2%	0.00659 g	0.01318 g	0.01978 g	0.03300 g	0.06616 g
5%	0.00263 g	0.00527 g	0.00790 g	0.01318 g	0.02638 g

✓ Pass: The determined minimum weight meets the requirement for the smallest net weight.

As Left Minimum Weight Table

Minimum weights for different weighing tolerances and safety factors					
Tolerance	Safety Factor				
	1	2	3	5	10
0.1%	0.12728 g	0.25614 g	0.38662 g	0.65256 g	1.34797 g
0.2%	0.06344 g	0.12728 g	0.19151 g	0.32118 g	0.65256 g
0.5%	0.02533 g	0.05072 g	0.07618 g	0.12728 g	0.25614 g
1%	0.01266 g	0.02533 g	0.03802 g	0.06344 g	0.12728 g
2%	0.00633 g	0.01266 g	0.01899 g	0.03167 g	0.06344 g
5%	0.00253 g	0.00506 g	0.00759 g	0.01266 g	0.02533 g

✓ Pass: The determined minimum weight meets the requirement for the smallest net weight.

At these net minimum weight values, the measurement uncertainty of the weighing device is equal to or less than 1/1 (no safety factor), 1/2, 1/3, 1/5, or 1/10 of the required tolerance. The values are calculated with $k = 2$ and based on the linear formula of the measurement uncertainty of the weighing device in use.

The safety factor for As Found is always 1. This implies no safety factor. As Found testing looks at the behavior of the instrument from the past until test occurred. For the past, it is necessary to know that the tolerance was met, but not the safety factor. The safety factor is a proactive measure to apply for future measurements.

Notes on minimum weight values in above table:

1. If "N/A" is shown above, no appropriate value could be calculated.
2. METTLER TOLEDO is not responsible for the definition of the process requirements.

Measurement Results

Results Summary

Repeatability		Eccentricity		Error of Indication	
As Found	✓	As Found	✓	As Found	✓
As Left	✓	As Left	✓	As Left	✓

✓ = Passed
✗ = Failed
i.e. = Safety Factor not met

Repeatability

Test Load: 100 g

Control Limit		As Found		As Left	
Tolerance	Result	Std. Deviation	Result	Std. Deviation	Result
0.1%	0.00050 g		✓		✓
0.2%	0.00100 g		✓		✓
0.5%	0.00250 g		✓		✓
1%	0.00500 g	0.00005 g	✓	0.00005 g	✓
2%	0.01000 g		✓		✓
5%	0.02500 g		✓		✓

The weighing tolerance is met if the standard deviation is less than or equal to the corresponding control limit.

Eccentricity

Test Load: 100 g

Control Limit		As Found		As Left	
Tolerance	Result	Deviation	Result	Deviation	Result
0.1%	0.0500 g		✓		✓
0.2%	0.1000 g		✓		✓
0.5%	0.2500 g		✓		✓
1%	0.5000 g	0.0001 g	✓	0.0001 g	✓
2%	1.0000 g		✓		✓
5%	2.5000 g		✓		✓

The weighing tolerance is met if the deviation is less than or equal to the corresponding control limit.

Error of Indication

As Found

		Control limits for various weighing tolerances							
Reference Value	Error	0.1%	0.2%	0.5%	1%	2%	5%		
0.0000 g	0.0000 g	N/A	N/A	N/A	N/A	N/A	N/A		
50.0000 g	-0.0003 g	0.0250 g	0.0500 g	0.1250 g	0.2500 g	0.5000 g	1.2500 g		
100.0000 g	-0.0005 g	0.0500 g	0.1000 g	0.2500 g	0.5000 g	1.0000 g	2.5000 g		
149.9999 g	-0.0006 g	0.0750 g	0.1500 g	0.3750 g	0.7500 g	1.5000 g	3.7500 g		
199.9998 g	-0.0008 g	0.1000 g	0.2000 g	0.5000 g	1.0000 g	2.0000 g	5.0000 g		
Result		✓	✓	✓	✓	✓	✓		✓

As Left

		Control limits for various weighing tolerances							
Reference Value	Error	0.1%	0.2%	0.5%	1%	2%	5%		
0.0000 g	0.0000 g	N/A	N/A	N/A	N/A	N/A	N/A		
50.0000 g	0.0001 g	0.0250 g	0.0500 g	0.1250 g	0.2500 g	0.5000 g	1.2500 g		
100.0000 g	0.0001 g	0.0500 g	0.1000 g	0.2500 g	0.5000 g	1.0000 g	2.5000 g		
149.9999 g	0.0001 g	0.0750 g	0.1500 g	0.3750 g	0.7500 g	1.5000 g	3.7500 g		
199.9998 g	0.0001 g	0.1000 g	0.2000 g	0.5000 g	1.0000 g	2.0000 g	5.0000 g		
Result		✓	✓	✓	✓	✓	✓		✓

The weighing tolerance is met if the error (of indication) for each test point is less than or equal to the corresponding control limit for that particular weighing tolerance. Results at or close to the zero point cannot be assessed.

COPY



CALIBRATION CERTIFICATE



Certificate No. : L202405022-0013

Date Issued : 08-May-24

Customer
 : Eastern Thai Consulting 1992 Co., Ltd.
 683 Moo 11, Sukhapibarn 8 Rd., Nongkham, Sriracha, Chonburi 20230

Equipment
 : Analog Barometer

Manufacturer
 : Barigo

Model
 : -

Serial No.
 : -

ID No./Tag No.
 : BM001/41

Date Received
 : 03-May-24

Date Calibrated
 : 06-May-24

Calibrated by
 : Mr. Saruth Srichulikul

Calibration Method or Calibration Procedure Used

In-house method : CP-21 base on DKD-R 6-1: Edition 3 2014.

This certificate is traceable to national standards, which realize the units of measurement according to the International System of Units (SI).

Result of Calibration

The reported uncertainty of measurement was based on standard uncertainty multiplied by a coverage factor $k = 2$, providing a level confidence approximately 95 percent.

This certificate may not be reproduced other than in full except with the prior written approval of the Miracle International Technology Company Limited.

Approved by: *Sarayuth T.*
 (Mr. Sarayuth Tochua)



Page 1 of 2

COPY

Certificate No : L202405022-0013

Environment
 Ambient Temperature : (25 ± 2)°C
 Relative Humidity : (50 ± 15%)RH

STD Reading mbar	UUC Reading (mbar) Before Adjusted	UUC Reading (mbar) After Adjusted	UUC Error mbar	Uncertainty ± mbar	MPE ± mbar	Pass / Fail with Guard Band
990.00	990	-	0.00	0.59	10.3	Pass
1000.00	1000	-	0.00	0.59	10.3	Pass
1010.00	1010	-	0.00	0.59	10.3	Pass
1020.00	1020	-	0.00	0.59	10.3	Pass
1030.00	1030	-	0.00	0.59	10.3	Pass

STD = Standard Pass = $|\text{error}| + |\text{uncertainty}| \leq |\text{MPE}|$

UUC = Unit Under Calibration Fail = $|\text{error}| + |\text{uncertainty}| > |\text{MPE}|$

MPE = Maximum Permissible Error

Calibrated condition :

Pressure Medium
 Mounting Position
 Reference Level
 Conversion Factor
 Air : Density = 1.19 kg/m³ @ 20°C, 1 bar
 Vertical
 at center of its dial
 Multiply by 1.0 E+02 - Pa unit

Description of UUC :

Range
 Calibration Range
 Scale Interval
 950 - 1080 mbar Absolute
 990 - 1030 mbar Absolute
 1 mbar

Condition As-Received : Used Item

The measurement results and statements of conformity with specification only relate to the item calibrated.

Measurement Standards Used & Traceability :

The International System of Units (SI) through

IRPC Certificate No. CL1-P230097 for Reference Pressure Monitor Serial No. 1598, Due 09-Nov-24

End of Certificate

Page 2 of 2

COPY

Results of Calibration

Resolution : 0.5 °C

1. Reporting of Temperature

Calibration point (°C)	UUC* setting (°C) reading (°C)	Measured temperature at each positions (°C)										Uncertainty ± (°C)	Coverage factor k
		# 1	# 2	# 3	# 4	# 5	# 6	# 7	# 8	# 9	# 10		
104	103.5	103.5	103.54	103.85	103.84	103.97	103.93	103.64	103.51	104.23		0.47	2.00

2. Characterization results

Calibration point (°C)	Stability ± (°C)	Uniformity (°C)	Overall variation (°C)
104	0.04	0.78	0.81

Notes

UUC* = Unit Under Calibration

[Signature]

Customer : EASTERN THAI CONSULTING 1992 CO., LTD.

683 Moo 11, Sukhapibarn 8 Rd., Nongkham,

Siracha, Chonburi 20230

Location of Calibration : EASTERN THAI CONSULTING 1992 CO., LTD.

(Hot Lab)

Equipment : Temperature controlled enclosures (Hot air oven)

Manufacturer : Memmert

Model : UFE 500

Serial No. : G511.0182

ID No. : LABE 17/4

Date of Receipt : 22 December 2023

Date of Calibration : 22 December 2023

Condition of Calibration

1. Environment

1.1 Ambient temperature : Maximum : 30.9 °C : Minimum : 29.6 °C

1.2 Relative humidity : Maximum : 54.5 % : Minimum : 46.8 %

1.3 Line voltage supplied : Maximum : 227.6 VAC : Minimum : 224.2 VAC

2. Calibration method

TLAS-G-20: Guidelines for calibration and checks of temperature controlled enclosures.

3. Reference standard instrument

Instrument : Data Acquisition With Sensor : LB-DA-08 (RTD-248 to RTD-256)

Certificate No. : 23-084070

Due Date : 06 August 2024

4. This certificate is traceable to the international system of unit (SI Unit).

The measurement is traceable to Asia Medical and Agricultural Laboratory and Research Center Public Company Limited.

5. This result of calibration was found accurate as shown on date and place of calibration only.

6. Condition of calibration item : Normal

Calibrated by : Mr. Pisek Into

Approved by : (Mr. Somchai Neampunt)

Scientist : Signed for Director

Issue date : 25 December 2023

The uncertainties are for a confidence probability of approximately 95%.

The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Asia Medical and Agricultural Laboratory and Research Center Public Company Limited (AMARC).

361 Soi Ladprao 122, Ladprao Road,

Phlabphla, Wang Thonglang, Bangkok 10310

Rev 01

TEL 02-516-2422

FAX 02-516-6949

Effective Date 15/10/21

CONTACT@AMARC.CO.TH

Customer : EASTERN THAI CONSULTING 1992 CO., LTD.

683 Moo 11, Sukhapibarn 8 Rd., Nongkham,

Siracha, Chonburi 20230

Location of Calibration : EASTERN THAI CONSULTING 1992 CO., LTD.

(Hot Lab)

Equipment : Temperature controlled enclosures (Hot air oven)

Manufacturer : Memmert

Model : UFE 500

Serial No. : G511.0182

ID No. : LABE 17/4

Date of Receipt : 22 December 2023

Date of Calibration : 22 December 2023

Condition of Calibration

1. Environment

1.1 Ambient temperature : Maximum : 30.9 °C : Minimum : 29.6 °C

1.2 Relative humidity : Maximum : 54.5 % : Minimum : 46.8 %

1.3 Line voltage supplied : Maximum : 227.6 VAC : Minimum : 224.2 VAC

2. Calibration method

TLAS-G-20: Guidelines for calibration and checks of temperature controlled enclosures.

3. Reference standard instrument

Instrument : Data Acquisition With Sensor : LB-DA-08 (RTD-248 to RTD-256)

Certificate No. : 23-084070

Due Date : 06 August 2024

4. This certificate is traceable to the international system of unit (SI Unit).

The measurement is traceable to Asia Medical and Agricultural Laboratory and Research Center Public Company Limited.

5. This result of calibration was found accurate as shown on date and place of calibration only.

6. Condition of calibration item : Normal

Calibrated by : Mr. Pisek Into

Approved by : (Mr. Somchai Neampunt)

Scientist : Signed for Director

Issue date : 25 December 2023

The uncertainties are for a confidence probability of approximately 95%.

The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Asia Medical and Agricultural Laboratory and Research Center Public Company Limited (AMARC).

361 Soi Ladprao 122, Ladprao Road,

Phlabphla, Wang Thonglang, Bangkok 10310

Rev 01

TEL 02-516-2422

FAX 02-516-6949

Effective Date 15/10/21

CONTACT@AMARC.CO.TH



REPORT OF CALIBRATION

Page 3 of 3

Certificate No. : 23-148804

Sample Code : 23-56200-006

NSC-TSI-TSI7025
CALIBRATION 0152

Results of Calibration

Notes

- Sensor installation locations
 - All sensors at any corners or walls should be positioned 5 cm (a x b x c) from the wall.
 - The reference sensor is preferably located of the geometric center of the chamber.
- Interior dimensions approx of chamber :
W = 56 cm ; D = 40 cm ; H = 48 cm
- Air valve or fresh air level : Off
- Fan level : Open
- The quoted uncertainty includes "Stability of chamber and loading effect in chamber at 20% of uniformity".
- Uniformity - the maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time.
- Stability - one-half of the greatest maximum difference of measured temperatures at any one sensor.
- Overall variation - the difference of the maximum and the minimum measured temperatures throughout observation time.
- UUC* reading - the average reading of indicating device that forms the integral part of the enclosure.
- Calibration results without adjustment.

The result expanded uncertainty of measurement U is stated as the standard uncertainty of measurement multiplied by the coverage factor k , which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty of measurement has been determined in accordance with IMAS M3003

- End of Report -

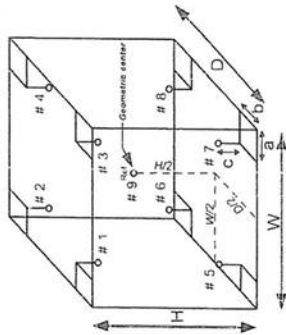


Figure: Example of sensor installation Positions

COPY



TISCH ENVIRONMENTAL, INC.
145 SOUTH MIAMI AVE
VILLAGE OF CLEVELAND, OH
45002
513.467.9000
877.283.7810 Toll Free
513.467.9009 FAX

ORIFICE TRANSFER STANDARD CERTIFICATION WORKSHEET TE-5025A

Date - Mar 24, 2016 Rootmeter S/N 0438320 Ta (K) - 295
Operator Tisch Orifice I.D. - 0136 Pa (mm) - 742.95

PLATE OR Run #	VOLUME START (m3)	VOLUME STOP (m3)	DIFF VOLUME (m3)	DIFF TIME (min)	METER DIFF Hg (mm)	ORIFICE DIFF H2O (in.)
1	NA	NA	1.00	1.3400	3.2	2.00
2	NA	NA	1.00	0.9510	6.3	4.00
3	NA	NA	1.00	0.8510	7.8	5.00
4	NA	NA	1.00	0.8130	8.6	5.50
5	NA	NA	1.00	0.6690	12.6	8.00

DATA TABULATION

(x axis) Qstd		(y axis)	(x axis) Qa		(y axis)
Vstd			Va		
0.9832	0.7337	1.4054	0.9957	0.7430	0.8911
0.9791	1.0296	1.9875	0.9915	1.0426	1.2603
0.9770	1.1481	2.2221	0.9894	1.1626	1.4090
0.9760	1.2006	2.3305	0.9884	1.2157	1.4778
0.9707	1.4510	2.8107	0.9830	1.4694	1.7823
Qstd slope (m) = 1.96262			Qa slope (m) = 1.22896		
intercept (b) = -0.03249			intercept (b) = -0.02060		
coefficient (r) = 0.99993			coefficient (r) = 0.99993		
Y axis = SQRT [H2O(Pa/760)] (298/Ta)]			Y axis = SQRT [H2O(Ta/Pa)]		

CALCULATIONS

Vstd = Diff. Vol [(Pa-Diff. Hg)/760] (298/Ta)
Qstd = Vstd/Time

Va = Diff Vol [(Pa-Diff Hg)/Pa]
Qa = Va/Time

For subsequent flow rate calculations:

Qstd = $1/m \{ [\text{SQRT} (\text{H}_2\text{O} (\text{Pa}/760) (298/\text{Ta}))] - b \}$
Qa = $1/m \{ [\text{SQRT} (\text{H}_2\text{O} (\text{Ta}/\text{Pa}))] - b \}$

COPY



CERTIFICATE OF CALIBRATION

Page 1 of 2
Certificate No. : 24-062442
Sample Code : 24-25546-002Customer : EASTERN THAI CONSULTING 1992 CO., LTD.
683 Moo 11, Sukhapibarn 8 Rd., Nongkharn,
Siracha, Chonburi 20230Location of Calibration : Asia Medical and Agricultural Laboratory and Research Center Public Company Limited
(Calibration laboratory)Equipment : Digital thermo-hygrometer
Manufacturer : testo Model : 608-H1
Serial No. : 45106737 ID No. : LABE 09/7
Date of Receipt : 23 May 2024 Date of Calibration : 27-28 May 2024

Condition of Calibration

1. Environment 1.1 Ambient temperature : 23.0 °C ± 3.0 °C
1.2 Relative humidity : 55.0 % ± 15.0 %

2. Calibration method

- 2.1 In-house method: WI-CL-045 By comparison with thermometer standard / chilled mirror hygrometer in controlled chamber.
2.2 The calibration by comparison unit under calibration (UUC) to the thermometer standard / chilled mirror hygrometer in a chamber at the controlled temperature / relative humidity.

3. Reference standard instrument

Instrument	Model	ID No.	Certificate No.	Due Date
3.1 Chilled Mirror	Optidew 401	LB-DP-03 & LB-DP-03 (DP)	TH-0064-23	07 August 2024
3.2 Digital Thermometer	Optidew 401	LB-DP-03 & LB-DP-03 (Temp.)	23-103423	03 September 2024
3.3 Digital Thermometer	34972A	LB-DA-07 with RTD-89	23-101374	05 September 2024

4. This certificate is traceable to the international system of unit (SI Unit).

4.1 Instrument No. 3.1 through National Institute of Metrology (Thailand).

4.2 Instrument No. 3.2 and 3.3 through Asia Medical and Agricultural Laboratory and Research Center Public Company Limited.

5. This result of calibration was found accurate as shown on date and place of calibration only.

6. Condition of calibration item : Normal

Calibrated by Miss Pornsuda Lohabal Scientist
Approved by (Mr. Somchai Neampunt) Signed for Director

Issue date 30 May 2024

The uncertainties are for a confidence probability of approximately 95%.

The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Asia Medical and Agricultural Laboratory and Research Center Public Company Limited (AMARC)



REPORT OF CALIBRATION

Page 2 of 2
Certificate No. : 24-062442
Sample Code : 24-25546-002

Results of Calibration

Temperature measurement

Resolution : 0.1 °C
Range : 0 °C to 50 °C

Calibration point °C	Average of standard reading		Unit under calibration		Expanded uncertainty °C
	Controlled humidity %RH	Temperature °C	Average reading °C	Correction value °C	
20	50	20.00	20.1	- 0.10	± 0.39
25	50	25.00	25.0	0.00	± 0.39
30	50	30.00	29.9	+ 0.10	± 0.39

Humidity measurement

Resolution : 0.1 %RH
Range : 10 %RH to 95 %RH

Calibration point %RH	Average of standard reading		Unit under calibration		Expanded uncertainty %RH
	Air temperature °C	Calculated humidity %RH	Average reading %RH	Correction value %RH	
45	25.02	45.10	48.4	- 3.30	± 1.3
60	25.01	60.07	63.4	- 3.33	± 1.5
75	25.01	75.15	78.5	- 3.35	± 1.7

Notes

Calibration results without adjustment.

The result expanded uncertainty of measurement U is stated as the standard uncertainty of measurement multiplied by the coverage factor k, which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty of measurement has been determined in accordance with UKAS M3003

- End of Report -

CERTIFICATE OF ANALYSIS

Grade of Product: EPA Protocol

Part Number: E04N199E15ACX9C Reference Number: 82-401135335-1
Cylinder Number: E80062815 Cylinder Volume: 144.4 CF
Laboratory: 124 - Riverton (SAP) - NJ Cylinder Pressure: 2015 PSIG
PGVP Number: B52018 Valve Outlet: 660
Gas Code: CO, NO, NOX, SO2, BALN Certification Date: Mar 13, 2018
Expiration Date: Mar 13, 2026

Certification performed in accordance with "EPA Traceability Protocol for Assay and Certification of Gaseous Calibration Standards (May 2012)" document EPA 600/R-12/531, using the assay procedures listed. Analytical methodology does not require correction for analytical interference. This cylinder has a total analytical uncertainty as stated below with a confidence level of 95%. There are no significant impurities which affect the use of this calibration mixture. All concentrations are on a volume/volume basis unless otherwise noted.

Do Not Use This Cylinder below 100 psig, i.e. 0.7 megapascals.

ANALYTICAL RESULTS					
Component	Requested Concentration	Actual Concentration	Protocol Method	Total Relative Uncertainty	Assay Dates
NOX	50.00 PPM	50.55 PPM	G1	+/- 1.4% NIST Traceable	03/06/2018, 03/13/2018
NITRIC OXIDE	50.00 PPM	50.50 PPM	G1	+/- 1.4% NIST Traceable	03/06/2018, 03/13/2018
SULFUR DIOXIDE	50.00 PPM	51.01 PPM	G1	+/- 1.0% NIST Traceable	03/06/2018, 03/13/2018
CARBON MONOXIDE	2000 PPM	1977 PPM	G1	+/- 1.0% NIST Traceable	03/06/2018
NITROGEN	Balance				

CALIBRATION STANDARDS			
Type	Lot ID	Cylinder No	Expiration Date
NTRM	16060607	CC442564	Jun 27, 2020
PRM	12367	APEX1099237	Jun 02, 2017
GMS	0315201604	CC503358	Jun 15, 2019
NTRM	16011025	CC473218	Jun 07, 2022
NTRM	12060735	CC356192	Dec 14, 2026

The SRM, PRM or RGM noted above is only in reference to the GMS used in the assay and not part of the analysis.

ANALYTICAL EQUIPMENT	
Instrument/Make/Model	Last Multipoint Calibration
Nicolet 6700 APW1100391 CO	FTIR
Nicolet 6700 APW1100391 NO	FTIR
Nicolet 6700 APW1100391 NO2	FTIR
Nicolet 6700 APW1100391 SO2	FTIR

Triad Data Available Upon Request

NOTES: NET WEIGHT: 10.43lbs

GROSS WEIGHT: 60.93lbs

PO# 5218000763

This calibration std. has been certified in accordance with the May 2012 EPA Traceability Protocol, Document EPA-600/R-12/531. All testing processes and measurements conform to the requirements of ISO/IEC 17025 and to Airgas ISO 9001:2000 and relate only to items identified on this certificate. All items are certified to be NIST Traceable with total uncertainty as detailed under Analytical Uncertainty. This document shall not be reproduced in full without written approval of the issuer.



TESTING CERT No. 3082.05

Donna Morris
Approved for Release

LA67-R 1075

Test Calibrated Report

Sulphur Dioxide Analyzer

Date : July 25, 2024

Time : 13:00

Model: API. M100E

Serial Number : 3138

Standard Gas : 51.65 PPM

Instrument Status

RANG (PPB)	500	DARK PMT (<50 mV)	26.9
STABIL (< 1 PPB)	0.501	DARK LAMP (< 50 mV)	0.000
SAMP PRESS (Ambient \pm 2 in-HG-A)	29.1	SLOPE (1.0 \pm 0.3)	0.975
SAMPLE FLOW (650 \pm 10 cc/min)	668	OFFSET (<100 mV)	23.9
PMT SIGNAL (0 \pm 100 mV)	35.7	HVPS (400-900 V)	739.0
NORM PMT (0 \pm 100 mV)	66.1	RCELL TEMP (50 C \pm 1)	50.0
UV LAMP (3500-4000mV)	2,965.8	BOX TEMP (Ambient \pm 5)	33.2
UV LAMP RATIO (%)	100.9	PMT TEMP (7 C \pm 2)	8.7
STR. LGT (<60 PPB)	11.655		
ETEST PMT Reading	OK		
SO2 Reading	OK		
OTEST PMT Reading	OK		
SO2 Reading	OK		

Calibrated Setting

Initial Reading (Before Adj.)		
Span Set Point	Concentration (PPB)	Analyzer Response (PPB)
Zero	0.0	0.00
Span	400.0	393.7

Final Reading (After Adj.)	Error %
Analyzer Response (PPB)	
0.00	-
400.1	0.03

RECEIVED

10 OCT 2024

Calibrated By :




LA67-R 1075

CALIBRATION MULTI-POINT OF SULFUR DIOXIDE ANALYZER

Station	ETC	Zero Setting	0
Brand	TELEDYNE API.	Span Instrument Gain	400.0
Model	M100E	Start time	13:00
Rang	500 PPB	Finish Time	15:00
Serial Number	3138	Date	July 25, 2024

SO ₂ Channel				
Point Number	Audit Concentration (PPB)	Analyzer Response (PPB)	Difference	
			(PPB)	(Percent)
ZERO	0	0.0	-	-
1	100	103.4	3.4	3.40
2	200	202.7	2.7	1.35
3	300	302.3	2.3	0.77
4	400	400.1	0.1	0.03
Average Difference (%)				1.39
Slope = 0.9991	Intercept = 1.88	Correlation Coefficient =	0.9999	

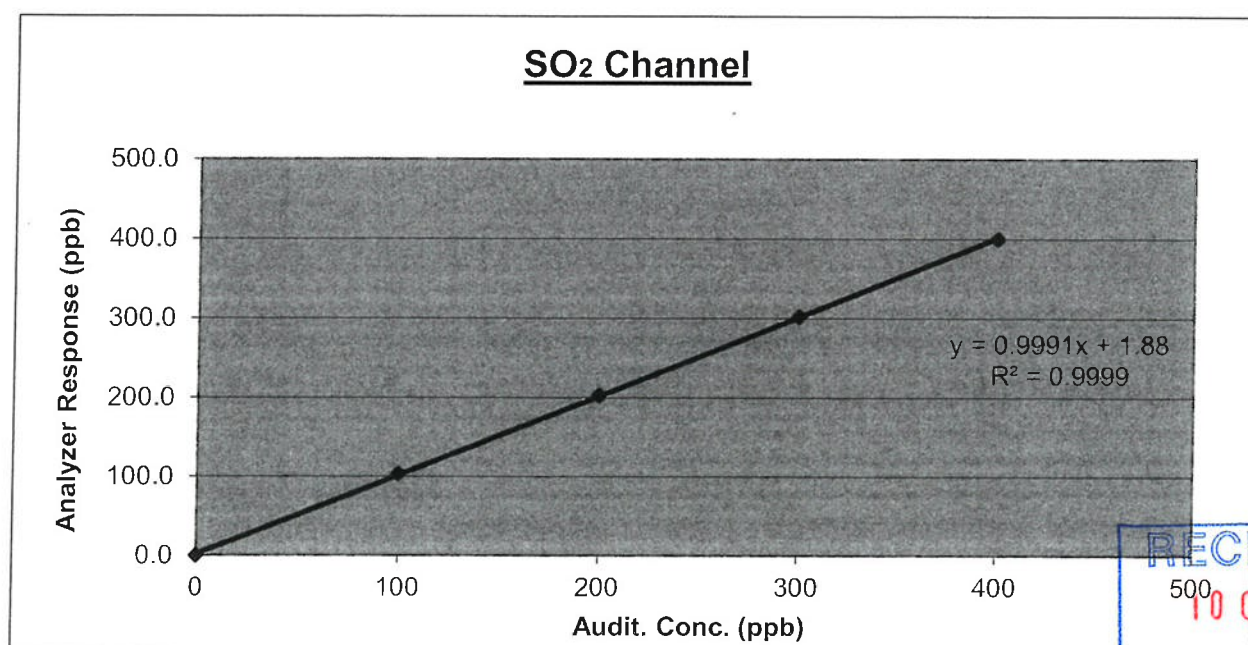

RECEIVED
500
10 OCT 2024

Signature

LA67-R 1075

Test Calibrated Report

Nitrogen Oxide Analyzer

Date : July 24, 2024

Time : 13:00

Model. API. T200

Serial Number : 7355

Standard Gas : 50.31 PPM

Instrument Status

Auto-Zero (-20 to 150 mV)	145.4	NO _x Offset (mV)	1.5
Box Temp.(Ambient Temp.plus 3-7)	34.8	NO _x Slope	1.007
HVPS (400 to 900 V.)	618	Nox Stabiliy (PPB to PPM)	0.02
Moly Temp. (315 +/-5)	314.4	O ₃ Flow (80 +/-15)	100.0
NO Norm Offset (mV)	0.4	PMT Signal (mV)	166.4
NO Slope	1.009	PMT Temp. (7 +/-2)	7.0
NO Stability (PPB to PPM)	0.03	R _x Cell Press (2-10 in-Hg-A)	6.4
NO ₂ Stability (PPB to PPM)	0.03	R _x Cell Temp. (50 +/-1)	50.0
Norm PMT (mV)	11.8	Sampe Flow (500 +/- 50)	492
Sample Press (in-Hg-A, Ambient)	28.6		

	PMT Reading	OK
ETEST	NO Conc Reading	OK
OPTIC TEST	NO _x Conc Reading	OK
	PMT Reading	OK
OTEST	NO Conc Reading	OK
	NO _x Conc Reading	OK

Calibrated Setting

Initial Reading (Before Adj.)		
Span Set Point	Concentration (PPB)	Analyzer Response (PPB)
Zero NO	0.0	0.00
Zero NO _x	0.0	0.00
Span NO	400.0	405.7
Span NO _x	401.0	408.8

Final Reading (After Adj.)	
Analyzer Response (PPB)	Error %
0.00	-
0.00	-
400.3	0.08
400.7	0.07

 RECEIVED
10 OCT 2024

Calibrated By :



LA67-R 1075

CALIBRATION MULTI-POINT OF NITROGEN OXIDE ANALYZER

Station	ETC	Zero Setting	0
Brand	TELEDYNE API.	Span Instrument Gain	400.0
Model	T200	Start time	13:00
Range	500 PPB	Finish Time	15:00
Serial Number	7355	Date	July 24, 2024

NO Channel				
Point Number	Audit Concentration (PPB)	Analyzer Response (PPB)	Difference	
			(PPB)	(Percent)
ZERO	0.0	0.0	-	-
1	100.0	102.6	2.6	2.60
2	200.0	202.9	2.9	1.45
3	300.0	300.8	0.8	0.27
4	400.0	400.3	0.3	0.08
Average Difference (%)				1.10
Slope = 0.9988		Intercept = 1.56		Correlation Coefficient = 0.9999

NOx Channel				
Point Number	Audit Concentration (PPB)	Analyzer Response (PPB)	Difference	
			(PPB)	(Percent)
ZERO	0.0	0.0	-	-
1	100.0	103.9	3.9	3.90
2	200.0	203.3	3.3	1.65
3	300.0	301.1	1.1	0.37
4	401.0	400.7	-0.3	0.07
Average Difference (%)				1.50
Slope = 0.9966		Intercept = 2.2818		Correlation Coefficient = 0.9999


RECEIVED

10 OCT 2024




LA67-R 1075

NO Channel

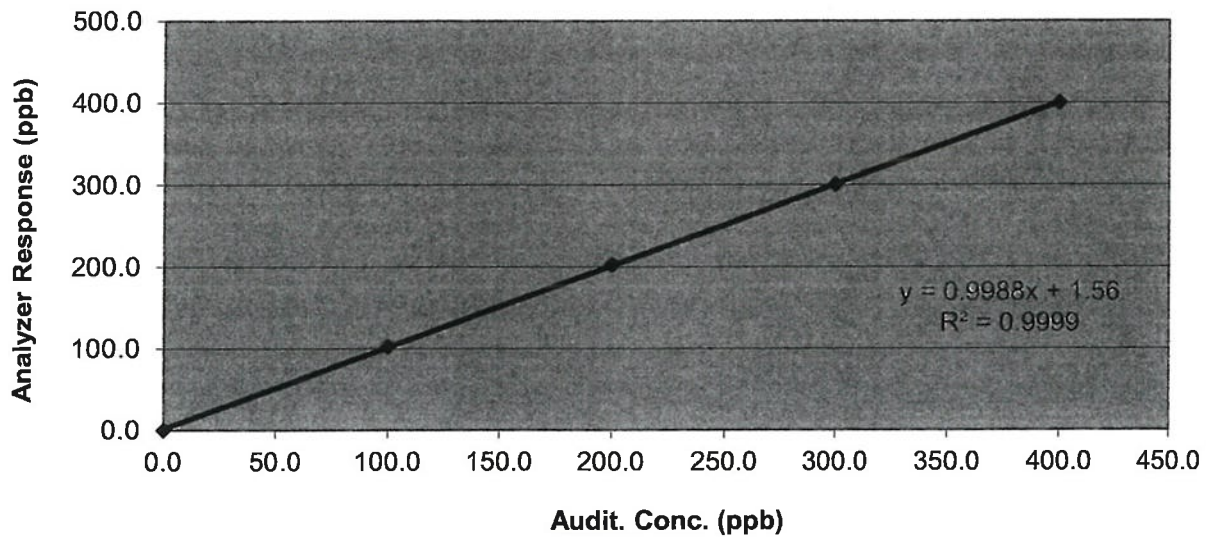

NO_x Channel

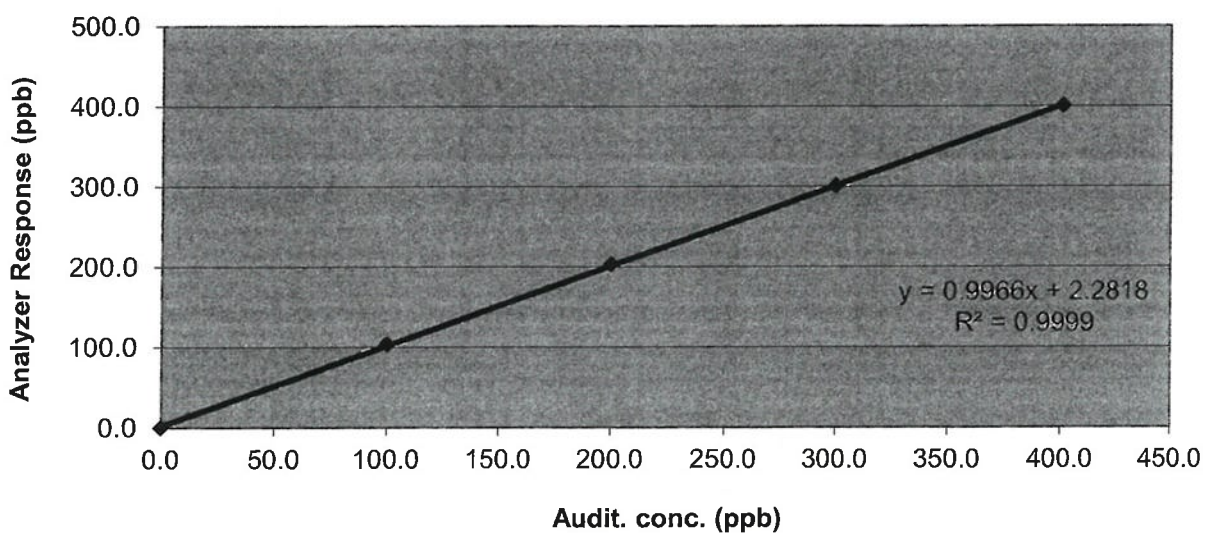

RECEIVED

10 OCT 2024



LA67-R 1075

Test Calibrated Report

Sulphur Dioxide Analyzer

Date : July 16, 2024

Time : 13:00

Model: APSA-370

Serial Number : 3XLWFYVJ

Standard Gas : 51.65 PPM

Instrument Status

Conc. Signal	16.1 mV
Light intensity	283.6 mV
Cell Temp.	39.0 C
5 V Power	5.0 V
24 V Power	24.0 V
Sample Flow Rate	700 cc/min
Pump Pressure	45.3 kPa
Atmospheric Pressure	101.0 kPa

Calibrated Setting

Initial Reading (Before Adj.)		
Span Set Point	Concentration (PPB)	Analyzer Response (PPB)
Zero	0.0	0.200
Span	400.0	396.7

Final Reading (After Adj.)	
Analyzer Response (PPB)	Error %
0.0	-
399.9	-0.03

Span SO2

0.94552

Calibrated By :

RECEIVED


10 OCT 2024



CALIBRATION MULTI-POINT OF SULFUR DIOXIDE ANALYZER

Station	ETC	Zero Setting	0
Brand	HORIBA	Span Instrument Gain	400.0
Model	APSA-370	Start time	13:00
Rang	500 PPB	Finish Time	15:00
Serial Number	3XLWFYVJ	Date	July 16, 2024

SO ₂ Channel				
Point Number	Audit Concentration (PPB)	Analyzer Response (PPB)	Difference	
			(PPB)	(Percent)
ZERO	0.0	0.0	-	-
1	100.0	101.9	1.9	1.90
2	200.0	202.5	2.5	1.25
3	300.0	300.3	0.3	0.10
4	400.0	399.9	-0.1	0.03
Average Difference (%)				0.82
Slope = 0.9982		Intercept = 1.28		Correlation Coefficient = 1

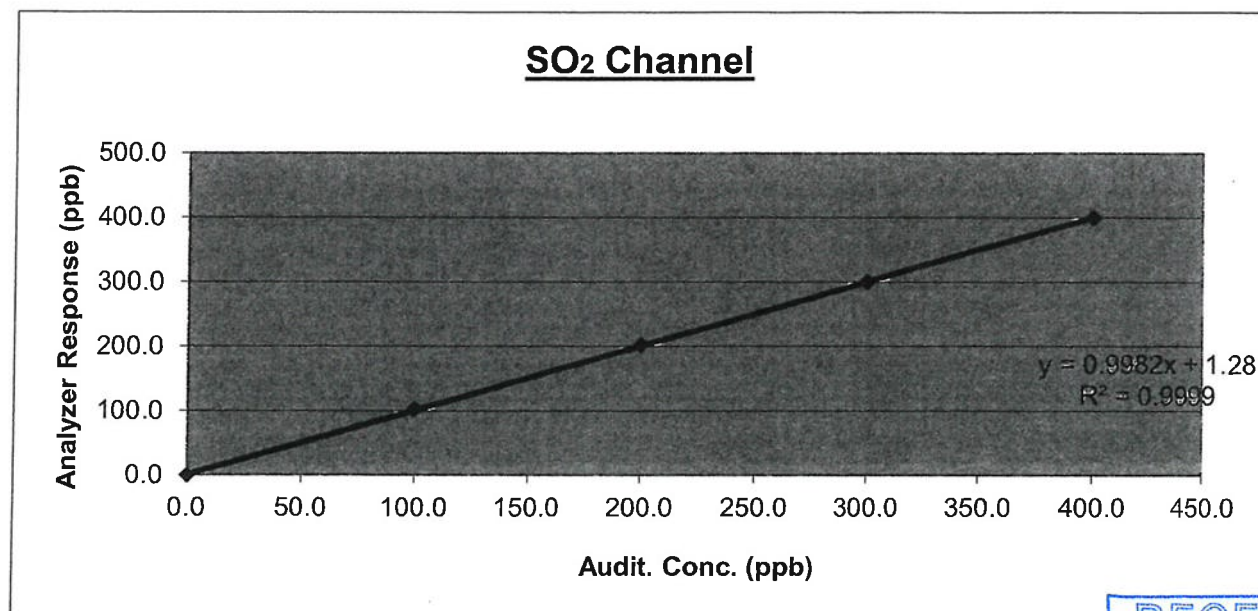

RECEIVED

10 OCT 2024



LA67-R1075

Test Calibrated Report

Nitrogen Oxide Analyzer

Date : August 23, 2024

Time : 13:00

Model.: APNA-370

Serial Number : XXSSJ4FM

Standard Gas : 50.31 PPM

Instrument Status

NOx Signal	6.7 mV
NO Signal	17.7 mV
Detector Temp.	40.4 C
5 V Power	5.0 V
24 V Power	23.7 V
Sample Flow Rate	700 cc/min
Pump Pressure	75.3 kPa
Atmospheric Pressure	101.2 kPa

Calibrated Setting

Initial Reading (Before Adj.)		
Span Set Point	Concentration (PPB)	Analyzer Response (PPB)
Zero NO	0.0	0.00
Zero NOx	0.0	0.00
Span NO	400	404.5
Span NOx	401	405.7

Final Reading (After Adj.)	
Analyzer Response (PPB)	Error %
0.0	-
0.0	-
400.2	0.05
401.1	0.02

Span NO 0.95408

Span NOx 0.93807

Calibrated By :

RECEIVED

10 OCT 2024



LA67-R1075

CALIBRATION MULTI-POINT OF NITROGEN OXIDE ANALYZER

Station	ETC	Zero Setting	0
Brand	HORIBA	Span Instrument Gain	400.0
Model	APNA-370	Start time	13:00
Range	500 PPB	Finish Time	15:00
Serial Number	XXSSJ4FM	Date	August 23, 2024

NO Channel				
Point Number	Audit Concentration (PPB)	Analyzer Response (PPB)	Difference	
			(PPB)	(Percent)
ZERO	0	0.0	-	-
1	100	103.6	3.6	3.60
2	200	202.4	2.4	1.20
3	300	302.4	2.4	0.80
4	400	400.2	0.2	0.05
Average Difference (%)				1.41
Slope = 0.9992		Intercept = 1.88		Correlation Coefficient = 0.9999

NOx Channel				
Point Number	Audit Concentration (PPB)	Analyzer Response (PPB)	Difference	
			(PPB)	(Percent)
ZERO	0	0.0	-	-
1	100	104.4	4.4	4.40
2	200	204.1	4.1	2.05
3	300	304.5	4.5	1.50
4	400	401.1	1.1	0.28
Average Difference (%)				2.06
Slope = 1.0023		Intercept = 2.36		Correlation Coefficient = 0.9998


RECEIVED

10 OCT 2024




LA67-R 1075

NO Channel

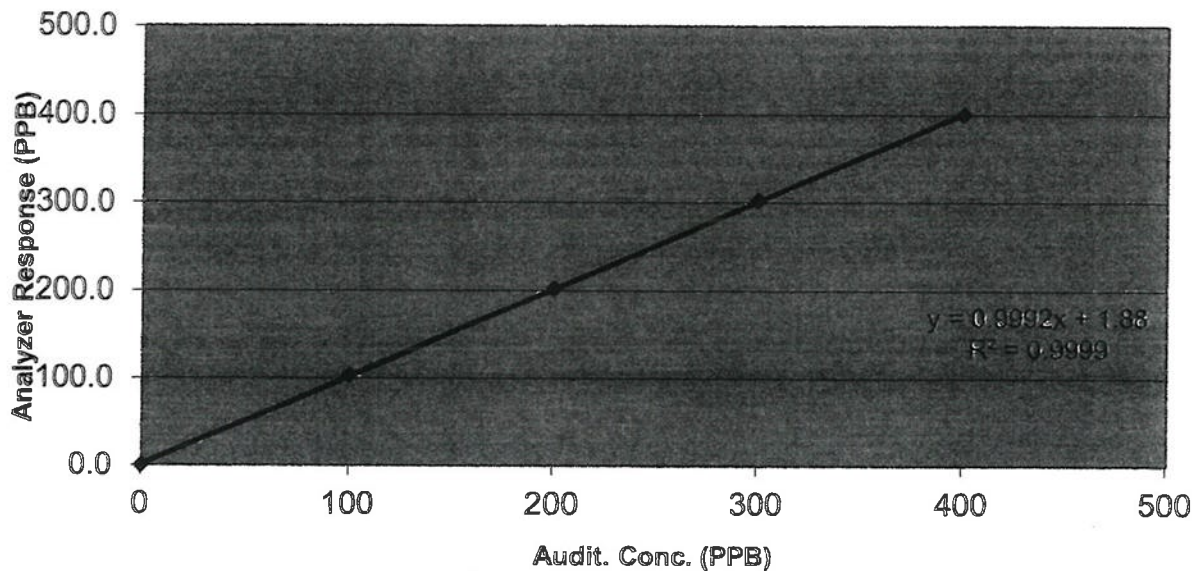

NO_x channel

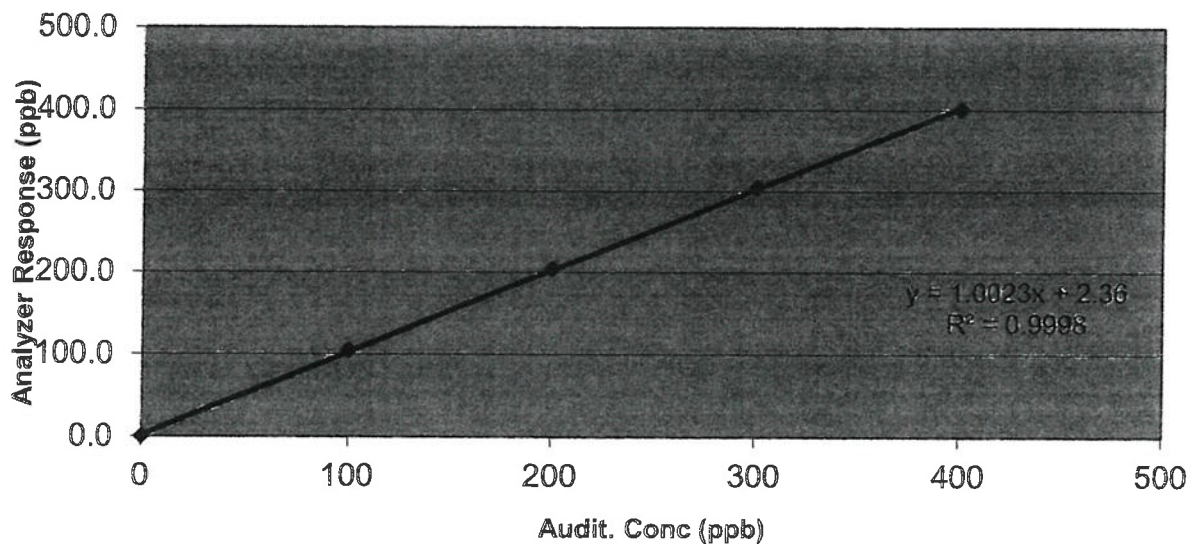

RECEIVED

10 OCT 2024

[Signature]

LA67-R 1075

Test Calibrated Report

Sulphur Dioxide Analyzer

Date : August 02, 2024

Time : 13:00

Model: API. M100E

Serial Number : 603

Standard Gas : 51.65 PPM

Instrument Status

RANG (PPB)	500	DARK PMT (<50 mV)	40.1
STABIL (< 1 PPB)	9.220	DARK LAMP (< 50 mV)	7.400
SAMP PRESS (Ambient+/-2 in-HG-A)	26.9	SLOPE (1.0 +/-0.3)	0.946
SAMPLE FLOW (650+/-10 cc/min)	663	OFFSET (<100 mV)	47.1
PMT SIGNAL (0+/-100 mV)	152.4	HVPS (400-900 V)	600.0
NORM PMT (0+/-100 mV)	131.6	RCELL TEMP (50 C +/-1)	50.0
UV LAMP (3500-4000mV)	3,507.0	BOX TEMP (Ambient +/- 5)	33.5
UV LAMP RATIO (%)	100.0	PMT TEMP (7 C +/-2)	8.1
STR. LGT (<60 PPB)	22.260		
ETEST PMT Reading	OK		
SO2 Reading	OK		
OTEST PMT Reading	OK		
SO2 Reading	OK		

Calibrated Setting

Initial Reading (Before Adj.)		
Span Set Point	Concentration (PPB)	Analyzer Response (PPB)
Zero	0.0	-3.98
Span	400.0	394.8

Final Reading (After Adj.)	
Analyzer Response (PPB)	Error %
0.0	-
400.4	0.10

RECEIVED

10 OCT 2024

Calibrated By :




LA67-R1075

CALIBRATION MULTI-POINT OF SULFUR DIOXIDE ANALYZER

Station	ETC	Zero Setting	0
Brand	TELEDYNE API.	Span Instrument Gain	400.0
Model	M100E	Start time	13:00
Rang	500 PPB	Finish Time	15:00
Serial Number	603	Date	August 02, 2024

SO ₂ Channel				
Point Number	Audit Concentration (PPB)	Analyzer Response (PPB)	Difference	
			(PPB)	(Percent)
ZERO	0.0	0.0	-	-
1	100.0	99.4	-0.6	0.60
2	200.0	201.6	1.6	0.80
3	300.0	300.1	0.1	0.03
4	400.0	400.4	0.4	0.10
Average Difference (%)				0.38
Slope = 1.0015		Intercept = 0.0		Correlation Coefficient = 1

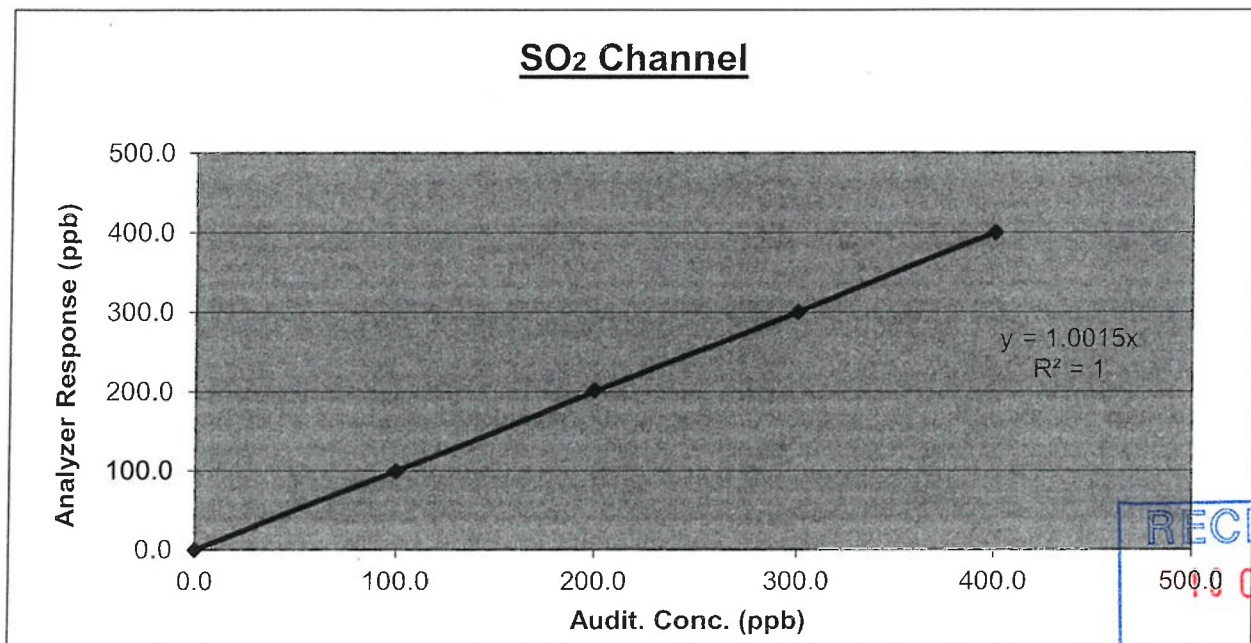

RECEIVED

19 OCT 2024



LA67-R 1075

Test Calibrated Report

Nitrogen Oxide Analyzer

Date : July 10 , 2024

Time : 13:00

Model. API. T200

Serial Number : 6757

Standard Gas : 50.31 PPM

Instrument Status

Auto-Zero (-20 to 150 mV)	-	NO _x Offset (mV)	355.1
Box Temp.(Ambient Temp.plus 3-7)	33.5	NO _x Slope	1.204
HVPS (400 to 900 V.)	607	Nox Stability (PPB to PPM)	0.67
Moly Temp. (315 +/-5)	313.6	O ₃ Flow (80 +/-15)	75.0
NO Norm Offset (mV)	351.6	PMT Signal (mV)	655.1
NO Slope	1.100	PMT Temp. (7 +/-2)	7.2
NO Stability (PPB to PPM)	0.26	R _x Cell Press (2-10 in-Hg-A)	3.1
NO ₂ Stability (PPB to PPM)	0.95	R _x Cell Temp. (50 +/-1)	50.00
Norm PMT (mV)	353.5	Sampe Flow (500 +/- 50)	470
Sample Press (in-Hg-A, Ambient)	28.4		

	PMT Reading	OK
ETEST	NO Conc Reading	OK
OPTIC TEST	NO _x Conc Reading	OK
	PMT Reading	OK
OTEST	NO Conc Reading	OK
	NO _x Conc Reading	OK

Calibrated Setting

Initial Reading (Before Adj.)		
Span Set Point	Concentration (PPB)	Analyzer Response (PPB)
Zero NO	0.0	2.08
Zero NO _x	0.0	-1.35
Span NO	400.0	410.7
Span NO _x	401.0	406.9

Final Reading (After Adj.)	
Analyzer Response (PPB)	Error %
0.00	-
0.00	-
400.1	0.03
400.8	0.05



10 OCT 2024

Calibrated By :



LA67-R 1075

CALIBRATION MULTI-POINT OF NITROGEN OXIDE ANALYZER

Station	ETC	Zero Setting	0
Brand	TELEDYNE API.	Span Instrument Gain	400.0
Model	T200	Start time	13:00
Range	500 PPB	Finish Time	15:00
Serial Number	6757	Date	July 10, 2024

NO Channel				
Point Number	Audit Concentration (PPB)	Analyzer Response (PPB)	Difference	
			(PPB)	(Percent)
ZERO	0.0	0.0	-	-
1	100.0	102.4	2.4	2.40
2	200.0	202.6	2.6	1.30
3	300.0	301.9	1.9	0.63
4	400.0	400.1	0.1	0.03
Average Difference (%)				1.09
Slope = 0.9997	Intercept = 1.46	Correlation Coefficient =	0.9999	

NOx Channel				
Point Number	Audit Concentration (PPB)	Analyzer Response (PPB)	Difference	
			(PPB)	(Percent)
ZERO	0.0	0.0	-	-
1	100.0	100.6	0.6	0.60
2	200.0	199.8	-0.2	0.10
3	300.0	300.7	0.7	0.23
4	401.0	400.8	-0.2	0.05
Average Difference (%)				0.25
Slope = 0.9997	Intercept = 0.2406	Correlation Coefficient =	1.0000	


RECEIVED

10 OCT 2024




LA67-R 1075

NO Channel

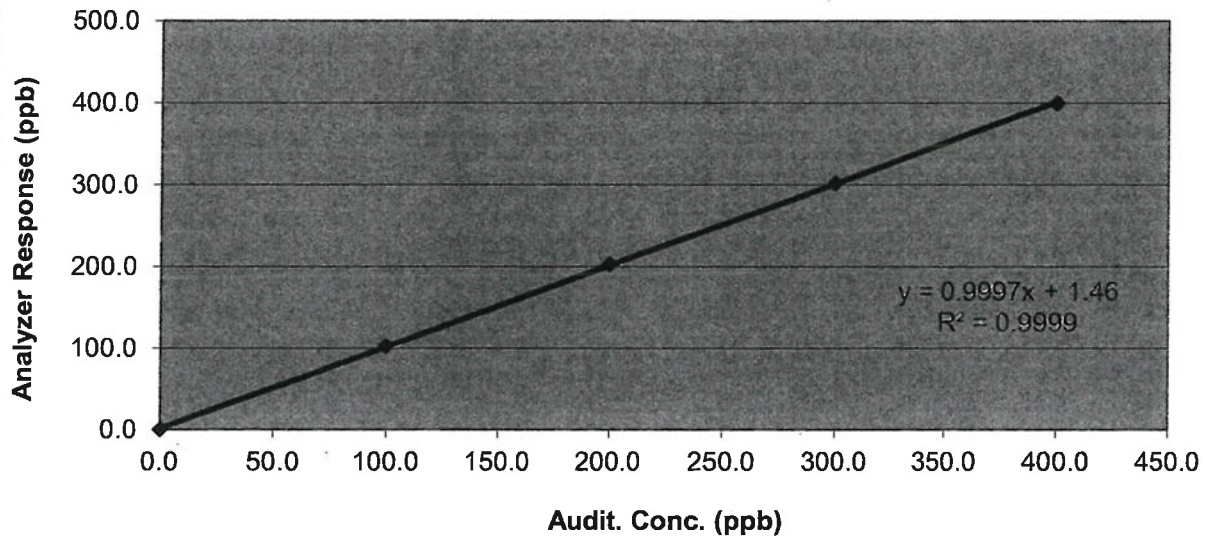

NO_x Channel

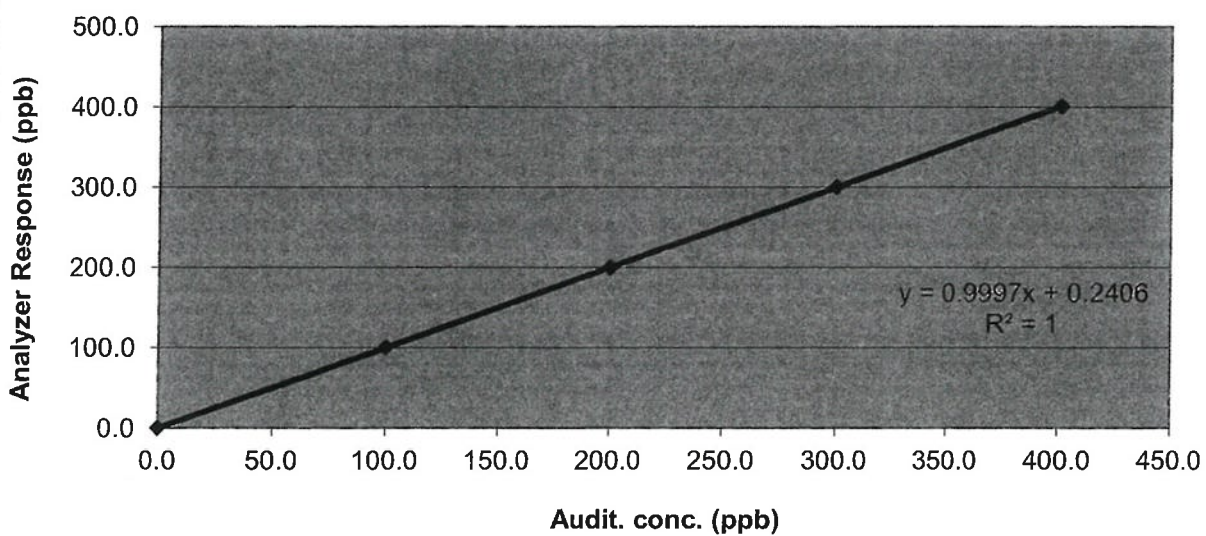

RECEIVED

10 OCT 2024



Certificate No. : 23-148799
Sample Code : 23-56200-001

CERTIFICATE OF CALIBRATION

Customer : EASTERN THAI CONSULTING 1992 CO., LTD.
683 Moo 11, Sukhapibarn 8 Rd., Nongkham,
Sriracha, Chonburi 20230

Location of Calibration : EASTERN THAI CONSULTING 1992 CO., LTD.
(Analytical Balance Room)

Equipment : ELECTRONIC BALANCE

Manufacturer : METTLER TOLEDO

Model : XS205DU

Serial No. : 1126323724

ID No. : LABE 05/1

Date of Receipt : 22 December 2023

Date of Calibration : 22 December 2023

Calibrated by : Mr. Somwang Sangdee
Scientist

Approved by : (Mr. Somchai Neampunt)
Signed for Director

Issue date : 25 December 2023

The uncertainties are for a confidence probability of approximately 95%.

The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Asia Medical and Agricultural Laboratory and Research Center Public Company Limited (AMARC).

REPORT OF CALIBRATION

Equipment : ELECTRONIC BALANCE
Manufacturer : METTLER TOLEDO
Model : XS205DU
Capacity : Max 81 g / 220 g
Resolution : 0.01 mg / 0.1 mg
Serial No. : 1126323724
ID No. : LABE 05/1

Result of Calibration

1. Test weight and repeatability of reading

Repeatability is a measure of the ability of a balance to supply the same result in repetitive weighings with one and the same load under the same measurement condition. The measurement of the repeatability must include both the balance specifications and the ambient (vibration, fluctuating air current/temperature/humidity, etc.) Operator handling of the balance is also included in the standard deviation.

Unit : g	Range : 80	<input checked="" type="checkbox"/> Before adjustment	<input checked="" type="checkbox"/> After adjustment
No adjustment	Nominal value	40	80
Adjustment	Standard weight	40.000054	80.000048
	Average reading of indicator	40.000026	80.000037
	Standard deviation	0.000015	0.000016
Unit : g	Range : 200	<input checked="" type="checkbox"/> Before adjustment	<input checked="" type="checkbox"/> After adjustment
No adjustment	Nominal value	100	200
Adjustment	Standard weight	100.000042	200.000041
	Average reading of indicator	100.00003	200.00004
	Standard deviation	0.000005	0.000003

COPY



Certificate No. : 23-148799

Sample Code : 23-56200-001

REPORT OF CALIBRATION

Result of Calibration

2. Sensitivity or value of a scale division

Change in the output variable of a measuring instrument divided by the associated change in the input variable.

Unit : g

Range : 80		Range : 200	
Test Point	Sensitivity, S	Test Point	Sensitivity, S
0	1.00748	0	1.0274
40	0.98753	100	0.9975
80	0.99751	200	0.9975

3. Departure of indication from nominal value, Linearity

Unit : g

Nominal Value	Standard Value	Average Reading of Indicator	Correction Value	Expanded Uncertainty	Coverage Factor (k)
Unload	0.0000000	0.00000	0.00000	0.000012	2.05
0.01	0.0100025	0.01000	0.00000	0.000012	2.05
0.1	0.1000019	0.10001	-0.00001	0.000013	2.03
1	1.0000125	1.00001	0.00000	0.000015	2.02
5	5.0000208	5.00004	-0.00002	0.000021	2.00
10	10.0000004	10.00008	-0.00008	0.000026	2.00
20	20.000030	20.00011	-0.00008	0.000036	2.00
50	50.0000014	50.00014	-0.00013	0.000068	2.00
100	100.000042	100.0001	-0.0001	0.00016	2.00
150	150.000056	150.0001	0.0000	0.00022	2.00
200	200.000041	200.0002	-0.0002	0.00027	2.00

The result expanded uncertainty of measurement U is stated as the standard uncertainty multiplied by the coverage factor k , which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty of measurement has been determined in accordance with UKAS M3003.

COPY



Certificate No. : 23-148799

Sample Code : 23-56200-001


REPORT OF CALIBRATION

Result of Calibration :

4. Eccentric or off-centre loading

Deviation of the measurement value through off - center (eccentric) loading. The corner load increases with the weight of the load and its removal from the center of the pan support.

Weighing pan ☐ Circle ☐ Triangular ☒ Rectangular
Test weight : 50 and 100
Unit : g

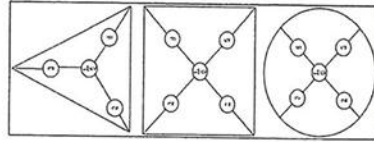

Range	Position	Reading of indicator	Reading of indicator	Test weight : 50 and 100 Unit : g
1	1	50.00015	100.0001	
2	2	50.00022	100.0001	
3	3	50.00008	100.0001	
4	4	50.00002	100.0000	
5	5	50.00016	100.0002	
6	6	50.00014	100.0001	
Maximum difference		0.00013	0.0001	

Condition of Calibration

1. Calibration Method : WI-CL-004 base on UKAS LAB 14: 2019
2. This result of calibration was found accurate as shown on date and place of calibration only.
3. Condition of Calibration item: Normal
4. This certification is traceable to the International System of Unit maintained at : -
Through the reference standard laboratory of Asia Medical and Agricultural Laboratory and Research Center Public Company Limited (Instrument number 1).
5. Reference standard instrument :

Instrument : STANDARD WEIGHT 1 mg to 1 kg
Class : E2
ID.No. : LB-WE-79
Certificate No. : 23-103642
Due Date : 10 September 2024

- End of Report -

COPY

CERTIFICATE OF ANALYSIS

Grade of Product: EPA Protocol

Part Number: E03N199E15AC0U4 Reference Number: 160-40224242-1
Cylinder Number: E801145030 Cylinder Volume: 144.4 CF
Laboratory: 124 - Plumsteadville - PA Cylinder Pressure: 2015 PSIG
PGVP Number: A12021 Valve Outlet: 350
Gas Code: CH4, PPN, BALN Certification Date: Oct 15, 2021

Expiration Date: Oct 15, 2029

Certification performed in accordance with "EPA Traceability Protocol for Assay and Certification of Gaseous Calibration Standards (May 2012)" document EPA 809/R-12/021, using the assay procedures listed. Analytical methodology does not require correction for any of the impurities listed. This cylinder has a full analytical uncertainty as stated below with a confidence level of 95%. There are no significant impurities which affect the use of this calibration mixture. All concentrations are on a mole/mole basis unless otherwise noted.

Do Not Use This Cylinder below 100 psig, i.e. 0.7 megapascals.

ANALYTICAL RESULTS				
Component	Requested Concentration	Actual Concentration	Protocol Method	Total Relative Uncertainty
METHANE	180.0 PPM	177.0 PPM	G1	+/- 1.0% NIST Traceable
PROpane	185.0 PPM	187.0 PPM	G1	+/- 1.0% NIST Traceable
NITROGEN	Balance			
Assay Dates				
				10/15/2021
				10/15/2021
CALIBRATION STANDARDS				
Type	Lot ID	Cylinder No	Concentration	Uncertainty
NTRM	08011503	K002564	246.7 PPM METHANE/AIR	+/- 0.6%
NTRM	200602-06	6162660Y	243.3 PPM PROPANE/AIR	+/- 0.5%
Expiration Date				
				May 15, 2025
				Mar 17, 2027
ANALYTICAL EQUIPMENT				
Instrument/Make/Model	Analytical Principle			
Nicolet IS50 FTIR AUP2110295 CH4	FTIR			
Nicolet IS50 FTIR AUP2110295 C3H8	FTIR			
Last Multipoint Calibration				
				Oct 13, 2021
				Oct 14, 2021

Triad Data Available Upon Request

NOTES:

Gross Weight: 28.0 Kg
Net Weight: 4.9 Kg
PO# 5221004861



COPY

Michael A. Huber

Approved for Release

Certificate Of Calibration

Method 5 Pre-Test Console Calibration - Cubic meter (m3)

Meter Console Information

Console Model: MC572V
 Console serial: 0504003
 DGM Model #: SK25EX
 DGM Serial #: 00009854

Calibration Condition

Cal Date: 22-Apr-24
 Due Date: 23-Apr-25
 Cal Report No: WDS-SV6704001
 Ambient Temp (°C): 25
 Pressure (mm Hg): 758
 Relative Humidity (%): 60

Factors/Conversion

Std. Temp (°K): 298
 Std. Pressure (mm Hg): 760
 K₁ (K/mm Hg): 0.3857

Reference Equipment

WTM Model: W-NKoDa-5B WTM Cal. Due Date: Dec. 2023
 WTM Serial: 600245 Gamma: 1.0000

UUT Meter (DGM)

Run Time (minutes)	DGM Orifice (mm H ₂ O)	Volume		Outlet Temp		Volume		Outlet Temp	
		Initial	Final	Initial	Final	Initial	Final	Initial	Final
15.00	13.0	144 5926	144 7699	26	27	60 06607	60 24392	29	28
10.00	25.0	144 8168	144 9795	27	27	60 29098	60 45472	27	27
8.00	50.0	145 0164	145 2002	28	28	60 49135	60 67317	29	27
7.00	80.0	145 2238	145 4291	28	28	60 69691	60 90186	29	28
5.00	120.0	145 4909	145 6692	28	29	60 96349	61 14145	27	26

Reference Meter (WTM)

Standardized Data

Test Meter		Reference Meter		Correction Factor		Flow Rate		
Std. Volume	Std. Flow Rate	Std. Volume	Std. Flow Rate	"Gamma"	Variation	Std & Corr	0.0212 SCMM	Variation
$V_{m(std)}$ (m ³)	$Q_{m(std)}$ (m ³ /min)	$V_{ref(std)}$ (m ³)	$Q_{ref(std)}$ (m ³ /min)	(Y)	(ΔY)	$Q_{m(std)corr}$	ΔH_p	$\Delta \Delta H_p$
0.173	0.012	0.173	0.012	0.997	0.003	0.012	43.309	-0.858
0.159	0.016	0.160	0.016	1.004	0.011	0.016	43.381	-0.787
0.179	0.022	0.176	0.022	0.984	-0.009	0.022	45.447	1.280
0.201	0.029	0.199	0.028	0.989	-0.005	0.028	44.202	0.035
0.175	0.035	0.174	0.035	0.994	0.000	0.035	44.497	0.330
				0.993	= Y Avg	44.167 = ΔH@ Avg		

Pass/Fail Result: Pass

Note: For Calibration Factor Y, the ratio of the reading of the calibration meter to the dry gas meter, acceptable tolerance of individual values from the average is ±0.02

Note: For ΔH_p, orifice pressure differential that equates to 0.75cfm (0.0212m³/min) at standard temperature and pressure, acceptable tolerance of individual values from the average is ±0.2inches (5.1mm) H₂O

Approved By: _____

(Patpasu Chaisana)
 Service Manager

Date: 22-Apr-24

COPY

Certificate of Calibration - Supplemental

METHOD 5 PRE-TEST CONSOLE CALIBRATION

Nomenclature

P₃ - Barometric Pressure
 DGM - Dry Gas Meter
 K₁ - Constant based on standard temp and press
 t - Run time, in minutes
 P_m - ΔH (Meter Pressure, gauge)
 V_m - Volume collected by test meter, corrected for STP
 Q_{m(std)} - Calculated flow rate of test meter
 K' - Critical orifice coefficient
 P_{ref} - Measured pressure of reference meter
 t_{ref} - Temperature measured in reference meter
 t_m - Temperature measured in test meter
 Y - Ratio of volume collected from test meter and orifice
 sc - Scaling Factor
 Counts_{sc} - Number of pulse counts, standardized
 Counts_{raw} - Number of raw pulse counts of a calibration run

Equations

$$V_{m(std)} = Y * K_1 \frac{P_{ref} - P_{sc}}{T_{ref}}$$

$$V_{m(std)} = Counts_{std} * Y_{sc(avg)}$$

$$Counts_{std} = K_1 \frac{Counts_{raw} * (P_{ref} + \frac{P_{sc}}{2})}{T_{ref}}$$

$$Q_{m(std)} = \frac{V_{m(std)}}{t}$$


$$Y_{sc} = \frac{V_{m(std)}}{Counts_{std}}$$

$$K_1 = \frac{T_{ref}}{P_{ref}}$$

$$Y = \frac{V_{m(std)}}{V_{ref(std)}}$$


$$V_{ref(std)} = \Delta H_p \frac{P_{ref} - 0.00116296 * P_{sc} + \frac{P_{sc}}{2}}{T_{ref}} \left(\frac{T_{ref}}{T_{ref} - t} \right)$$

Calibration Train

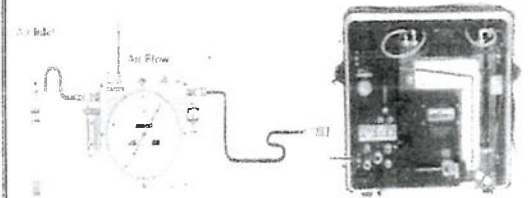


Calibration Graphs

Meter Pressure vs Flowrate

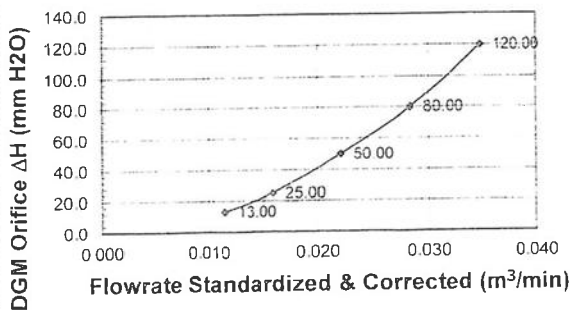

Console Serial: 0504003 Console Model: MC572V

Meter Gamma vs Flowrate

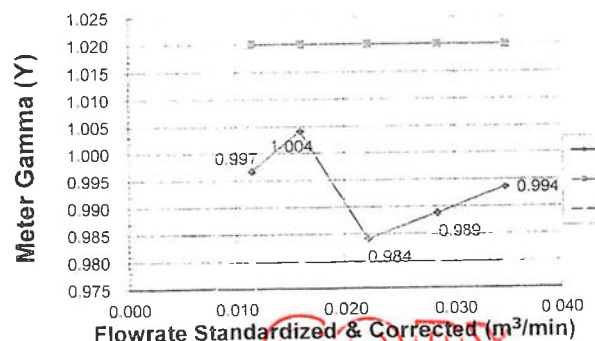

Console Serial: 0504003 Console Model: MC572V



WISDOM SCIENCE

TEMPERATURE DISPLAY CALIBRATION

Meter Console Information

Console Model	MC572V
Console serial	0504003
Temp Indicator Model	785-KF
Temp Indicator Serial	JC05630

Calibration Conditions

Cal Date	22-Apr-24
Due Date	23-Apr-25
Cal Report No	WDS-SV6704001
Ambient Temp (°C)	25
Pressure (mm Hg)	759
Humidity (%)	60

Reference Equipment

Temp Meter Model	Fluke 714B
Serial No	60590035
Cal Date	07-Apr-24
Temp Meter Model	Fluke 179
Serial No	58620112
Cal Date	06-Feb-24

Temperature Sensor Calibration

Reference Point	Ref Thermometer Temperature °C	Thermocouple Display Temperature °C	Temperature Difference °C
#			
1	-18.0	-17.0	1.0
2	38.0	37.0	1.0
3	93.0	93.0	0.0
4	149.0	150.0	-1.0
5	260.0	259.0	1.0
6	371.0	372.0	-1.0
7	482.0	492.0	0.0
8	593.0	591.0	0.0
9	815.0	815.0	1.0
10	1038.0	1038.0	0.0
Maximum ¹			1.0

Note

¹ For valid test results, the maximum difference between temperature readings should $\leq 1.0^{\circ}\text{C}$ (EPA Method 5, Section 6.1.1.8) Perform all TC Channel calibrations. Except meter (DGM) channel

PASS

DGM Out Temperature Sensor Calibration

Temperature point	Ref Thermometer Temperature °C	Thermocouple Display Temperature °C	Temperature Difference °C
#			
Ice	0.0	1.0	-1.0
Ambient	26.5	26.0	0.5
Heat	109.3	110.0	0.7

Temp Difference $\pm 2^{\circ}\text{F}$ or $\pm 1^{\circ}\text{C}$

PASS

Note

The temperatures of the thermocouple and reference thermometers shall agree to within $\pm 2^{\circ}\text{F}$ (EPA Method 5, section 10.5)

Approved By :

(Pelpasu Chaisana)

Service Manager

WISDOM SCIENCE

COPY



WISDOM SCIENCE

Certificate Of Calibration

Method 5 Pre-Test Console Calibration - Cubic meter (m3)

Meter Console Information

Console Model : XC-572-OV
 Console serial : A2204323
 DGM Model #: SK25EX
 DGM Serial #: 00008294

Calibration Condition

Cal. Date: 22-May-24
 Due Date: 22-May-25
 Cal. Report No.: WDS-SV6704018
 Ambient Temp (°C): 25
 Pressure (mm Hg): 758
 Relative Humidity (%): 60

Factors/Conversion

Std Temp (°K): 298
 Std. Pressure (mm Hg): 760
 K₁ (K/mm Hg): 0.3857

Reference Equipment

WTM Model: W-NKoDa-SB WTM Cal. Due Date: Dec. 2024
 WTM Serial: 600245 Gamma: 1.0000

UUT Meter (DGM)

Reference Meter (WTM)

Run Time (minutes)	DGM Orifice (mm H ₂ O)	Volume		Outlet Temp		Volume		Outlet Temp	
		Initial	Final	Initial	Final	Initial	Final	Initial	Final
9	P _{avg}	V _{in}	V _{out}	t _{in}	t _{out}	V _{in}	V _{out}	t _{in}	t _{out}
15.00	13.0	194.6567	194.8274	26	27	61.39400	61.56423	28	27
10.00	25.0	195.0941	195.2514	28	28	61.82541	61.98088	29	28
8.00	50.0	195.2786	195.4572	28	28	62.00769	62.10342	28	27
7.00	80.0	195.4877	195.6846	28	29	62.21353	62.40748	28	27
5.00	120.0	195.7085	195.8796	29	29	62.43108	62.60020	26	27

Standardized Data

Calibration Results

Test Meter		Reference Meter		Correction Factor		Flow Rate		ΔH (mm H ₂ O)	
Std. Volume	Std. Flow Rate	Std. Volume	Std. Flow Rate	"Gamma"	Variation	Std & Corr	0.0212 SCMM	Variation	
V _{avg} (m ³)	Q _{avg} m ³ /min	V _{avg} (m ³)	Q _{avg} m ³ /min	(Y)	(ΔY)	Q _{avg} m ³ /min	ΔH _{avg}	ΔH _{avg}	
0.167	0.011	0.166	0.011	0.994	0.008	0.011	47.022	-1.348	
0.153	0.015	0.151	0.015	0.986	0.000	0.015	48.311	-0.059	
0.174	0.022	0.171	0.021	0.981	-0.005	0.021	48.458	0.089	
0.192	0.027	0.189	0.027	0.981	-0.004	0.027	48.869	0.499	
0.167	0.033	0.165	0.033	0.986	0.000	0.033	49.189	0.819	
				0.985	Y Avg			48.370	ΔH @ Avg

Pass/Fail Result: Pass

Note: For Calibration Factor Y, the ratio of the reading of the calibration meter to the dry gas meter, acceptable tolerance of individual values from the average is ±0.02

Note: For ΔH_{avg}, orifice pressure differential that equates to 0.75cm (0.0212m³/min) at standard temperature and pressure, acceptable tolerance of individual values from the average is ±0.2inches (5.1mm) H₂O

Approved By:

(Palpasu Chaisana)
Service Manager

Date: 22-May-24

WISDOM SCIENCE
 บริษัท วิสโดม ไซนซ์ จำกัด
 WISDOM SCIENCE SALE AND SERVICE GROUP COMPANY LIMITED

COPY

Certificate of Calibration - Supplemental

METHOD 5 PRE-TEST CONSOLE CALIBRATION

Nomenclature

Equations

Calibration Train

P_B - Barometric Pressure
 DGM - Dry Gas Meter
 K₁ - Constant based on standard temp and press
 t - Run time, in minutes
 P_m - ΔH (Meter Pressure, gauge)
 V_m - Volume collected by test meter, corrected for STP
 Q_m - Calculated flow rate of test meter
 K' - Critical orifice coefficient
 P_w - Measured pressure of reference meter
 t_w - Temperature measured in reference meter
 t_m - Temperature measured in test meter
 Y - Ratio of volume collected from test meter and orifice
 sc - Scaling Factor
 Counts_{std} - Number of pulse counts, standardized
 Counts_{std} - Number of raw pulse counts of a calibration run

$$V_{m(std)} = Y * K_1 \frac{V_w * (P_{bar} + \frac{P_{m(std)}}{1.36})}{T_w}$$


$$V_{m(std)} = Counts_{std} * Y_{sc(avg)}$$

$$Counts_{std} = K_1 \frac{Counts * (P_{bar} + \frac{P_{m(std)}}{1.36})}{T_w}$$

$$Q_{m(std)} = \frac{V_{m(std)}}{t}$$


$$K_1 = \frac{T_{std}}{P_{std}} * Y = \frac{V_{m(std)}}{V_{m(std)}}$$

$$Y = \frac{P_{m(std)} + 0.0011696 * P_{m(std)} * \frac{P_{m(std)}}{1.36}}{P_{std}} * \left(\frac{T_{std}}{T_w} \right)$$

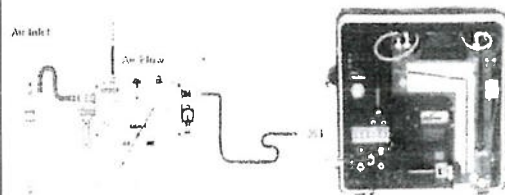


Calibration Graphs

Meter Pressure vs Flowrate

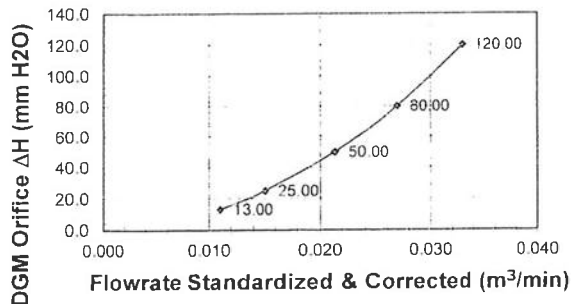

Meter Gamma vs Flowrate

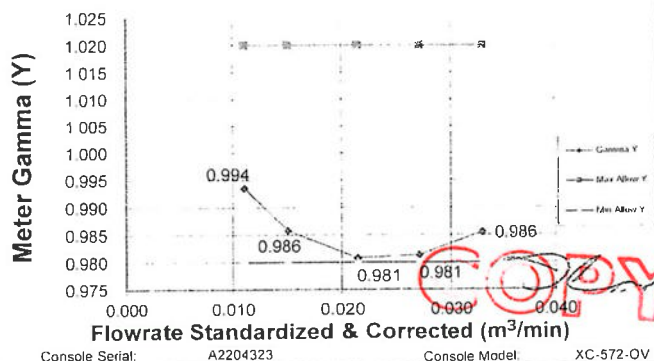



WISDOM SCIENCE

TEMPERATURE DISPLAY CALIBRATION

Meter Console Information

Console Model	XC-572-OV
Console serial	A2204323
Temp Indicator Model	755-KF
Temp Indicator Serial	JC05630

Calibration Conditions

Cal Date	22-May-24
Due Date	22-May-25
Cal Report No	WDS-SVP704018
Ambient Temp (°C)	25
Pressure (mm Hg)	758
Humidity (%)	60

Reference Equipment

Temp Meter Model	Fuke 714B
Serial No	60590035
Cal Date	07-Apr-24
Temp Meter Model	Fuke 179
Serial No	58620112
Cal Date	06-Feb-24

Temperature Sensor Calibration

Reference Point	Ref Thermometer Temperature	Thermocouple Display Temperature	Temperature Difference
#	°C	°C	°C
1	-18.0	-17.0	1.0
2	38.0	37.0	1.0
3	93.0	93.0	0.0
4	149.0	150.0	-1.0
5	260.0	255.0	5.0
6	371.0	372.0	-1.0
7	482.0	482.0	0.0
8	593.0	593.0	0.0
9	815.0	815.0	0.0
10	1036.0	1033.0	3.0
Maximum ¹			1.0

Note

¹ For valid test results, the maximum difference between temperature readings should be $\leq 1.0^{\circ}\text{C}$ (EPA Method 5, Section 6.1.8)
Perform all TC Channel calibrations. Except meter (DGM) channel

PASS

DGM Out Temperature Sensor Calibration

Temperature point	Ref Thermometer Temperature	Thermocouple Display Temperature	Temperature Difference
#	°C	°C	°C
Ice	0.0	1.0	-1.0
Ambient	27.5	27.0	0.5
Heat	108.6	105.0	3.6

Difference Range

Temp. Difference $\pm 2^{\circ}\text{F}$ or $\pm 1^{\circ}\text{C}$

PASS

Note

The temperatures of the thermocouple and reference thermometers shall agree to within $\pm 2^{\circ}\text{F}$ (EPA Method 5, section 10.5)

Approved By :

Patpasu Chaisana

(Patpasu Chaisana)

Service Manager

WISDOM SCIENCE

บริษัท วิสโดม ไซนซ์ จำกัด
WISDOM SCIENCE SALE AND SERVICE GROUP COMPANY LIMITED

COPY

Certificate Of Calibration

Method 5 Pre-Test Console Calibration - Cubic meter (m3)

Meter Console Information

Console Model : XC-572-V
Console serial : 1110070
DGM Model #: SK25EX
DGM Serial #: 00006432

Calibration Condition

Cal. Date: 28-Jun-24
Due Date: 28-Jun-25
Cal. Report No.: WDS-SV6706007
Ambient Temp (°C): 25
Pressure (mm Hg): 758
Relative Humidity (%): 60

Factors/Conversion

Std. Temp. (°K): 298
Std. Pressure (mm Hg): 760
K_f (K/mm Hg): 0.3857

Reference Equipment

WTM Model: W-NKoDa-5B WTM Cal. Due Date: Dec. 2024
WTM Serial: 600245 Gamma: 1.0000

UUT Meter (DGM)

Run Time (minutes)	DGM Orifice (mm H ₂ O)	Volume		Outlet Temp		Volume		Outlet Temp	
		Initial	Final	Initial	Final	Initial	Final	Initial	Final
0	P _{m(st)}	V _{mi}	V _{mf}	t _{mi}	t _{mf}	V _{wi}	V _{wf}	t _{wi}	t _{wf}
15.00	13.0	239.7603	239.9212	27	27	63.63889	63.79843	27	27
10.00	25.0	239.9406	240.0979	27	27	63.81777	63.97353	27	27
8.00	50.0	240.1147	240.2952	27	28	63.99028	64.16968	26	26
7.00	80.0	240.3308	240.5352	28	28	64.20536	64.40956	26	26
5.00	120.0	240.5641	240.7422	29	29	64.43852	64.61730	26	26

Standardized Data

Test Meter		Reference Meter		Correction Factor		Flow Rate		ΔH@ (mm H ₂ O)	
Std. Volume	Std. Flow Rate	Std. Volume	Std. Flow Rate	"Gamma"	Variation	Std & Corr	ΔH _g	Variation	ΔΔH _g
V _{m(std)} (m ³)	Q _{m(std)} m ³ /min	V _{w(std)} (m ³)	Q _{w(std)} m ³ /min	(Y)	(ΔY)	Q _{m(std)corr}	ΔH _g		
0.157	0.010	0.155	0.010	0.991	-0.003	0.010	53.303	6.250	
0.154	0.015	0.152	0.015	0.989	-0.005	0.015	47.860	0.807	
0.176	0.022	0.175	0.022	0.993	-0.001	0.022	46.233	-0.820	
0.200	0.029	0.199	0.028	0.997	0.003	0.028	43.895	-3.158	
0.174	0.035	0.175	0.035	1.001	0.007	0.035	43.973	-3.080	
				0.994	= Y Avg.		47.053	= ΔH@ Avg.	

Pass/Fail Result: **Pass**

Note: For Calibration Factor Y, the ratio of the reading of the calibration meter to the dry gas meter, acceptable tolerance of individual values from the average is ±0.02.

Note: For ΔH_g, orifice pressure differential that equates to 0.75cfm (0.0212m³/min) at standard temperature and pressure, acceptable tolerance of individual values from the average is ±0.2inches (5.1mm) H₂O.

Approved By:

Patras Chaisana
(Patras Chaisana)
Service Manager

WISDOM SCIENCE

บริษัท วิสโดม ไซนส์ แอนด์ เซอร์วิส จำกัด
WISDOM SCIENCE SALE AND SERVICE GROUP COMPANY LIMITED

Date

28-Jun-24

COPY

Certificate of Calibration - Supplemental

METHOD 5 PRE-TEST CONSOLE CALIBRATION

Nomenclature

P_a - Barometric Pressure
DGM - Dry Gas Meter
K_f - Constant based on standard temp and press
θ - Run time, in minutes
P_m - ΔH (Meter Pressure, gauge)
V_m - Volume collected by test meter, corrected for STP
Q_{m(std)} - Calculated flow rate of test meter
K' - Critical orifice coefficient
P_w - Measured pressure of reference meter
t_w - Temperature measured in reference meter
t_m - Temperature measured in test meter
Y - Ratio of volume collected from test meter and orifice
sc - Scaling Factor
Counts_{std} - Number of pulse counts, standardized
Counts_{total} - Number of raw pulse counts of a calibration run

Equations

$$V_{w(std)} = Y * K_1 \frac{V_w * (P_{bar} + \frac{P_{m(std)}}{13.6})}{T_w}$$

$$V_{m(std)} = Counts_{std} * Y_{sc(avg)}$$


$$Counts_{std} = K_1 \frac{Counts_{total} * (P_{bar} + \frac{P_{m(std)}}{13.6})}{T_m}$$

$$Q_{w(std)} = \frac{V_{w(std)}}{\theta} \quad Y_{sc} = \frac{V_{m(std)}}{Counts_{std}}$$

$$K_1 = \frac{T_{std}}{P_{std}} \quad Y = \frac{V_{m(std)}}{V_{w(std)}}$$


$$Metric \Delta H_g = \frac{P_{m(std)} + 0.0011629 * (P_{m(std)} + \frac{P_{m(std)}}{13.6})}{T_{std}} * \left(\frac{T_w + \theta}{T_w + P_{std}} \right)$$

Calibration Train

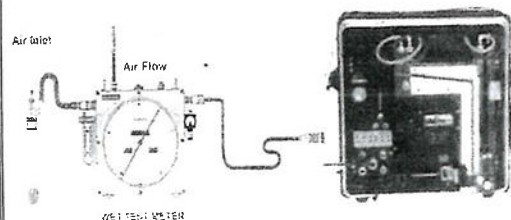

Calibration Graphs


Meter Pressure vs Flowrate

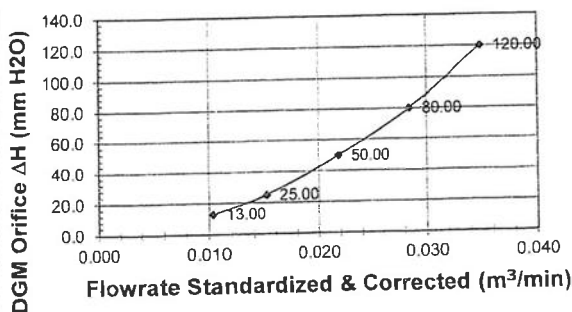

Console Serial: 1110070

Console Model: XC-572-V

Meter Gamma vs Flowrate

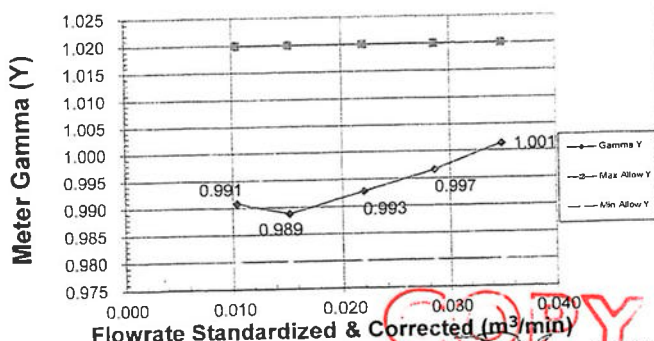

Console Serial: 1110070

Console Model: XC-572-V



WISDOM SCIENCE

TEMPERATURE DISPLAY CALIBRATION

Meter Console Information

Console Model : XC-572-V
 Console serial : 1110070
 Temp Indicator Model : ID-85
 Temp Indicator Serial :

Calibration Conditions

Cal Date : 28-Jun-24
 Due Date : 28-Jun-25
 Cal. Report No. : WDS-SV6706007
 Ambient Temp. (°C) : 25
 Pressure (mm Hg) : 756
 Humidity (%) : 60

Reference Equipment

Temp. Meter Model : Fluke 71-4B
 Serial No. : 60590035
 Cal. Date : 07-Apr-24
 Temp. Meter Model : Fluke 17g
 Serial No. : 59620112
 Cal. Date : 06-Feb-24

Temperature Sensor Calibration

Reference Point	Ref. Thermometer Temperature °C	Thermocouple Display Temperature °C	Temperature Difference °C
#			
1	-18.0	-17.0	1.0
2	38.0	39.0	-1.0
3	93.0	94.0	-1.0
4	148.0	150.0	-1.0
5	280.0	281.0	-1.0
6	371.0	372.0	-1.0
7	482.0	483.0	-1.0
8	593.0	593.0	0.0
9	816.0	815.0	1.0
10	1038.0	1038.0	0.0
Maximum			1.0

Note

* For valid test results, the maximum difference between temperature readings should $\leq 1.0^{\circ}\text{C}$ (EPA Method 5, Section 6.1.1.8).
 Perform all TC Channel calibrations. Except meter (DGM) channel

PASS

DGM Out Temperature Sensor Calibration

Temperature point	Ref. Thermometer Temperature °C	Thermocouple Display Temperature °C	Temperature Difference °C
#			
Ice	1.0	2.0	-1.0
Ambient	24.2	25.0	-0.8
Heat	110.5	111.0	-0.5

Difference Rang

Temp. Difference $\pm 2^{\circ}\text{F}$ or $\pm 1^{\circ}\text{C}$

PASS

Note

The temperatures of the thermocouple and reference thermometers shall agree to within $\pm 2^{\circ}\text{F}$ (EPA Method 5, section 10.5)

Approved By :

(Signature)

(Paipasu Chaisana)

Service Manager

WISDOM SCIENCE

บริษัท วิสโดม ไซนซ์ จำกัด
 WISDOM SCIENCE SALE AND SERVICE GROUP COMPANY LIMITED

COPY

Certificate Of Calibration

Method 5 Pre-Test Console Calibration - Cubic meter (m3)

Meter Console Information

Console Model : MC-572-V
 Console serial : 1007055
 DGM Model #: SK25EX
 DGM Serial #: 0009799

Calibration Condition

Cal. Date: 04-Aug-24
 Due Date: 04-Aug-25
 Cal. Report No.: WDS-SV6707001
 Ambient Temp (°C): 25
 Pressure (mm Hg): 758
 Relative Humidity (%): 60

Factors/Conversion

Std. Temp. (°K): 298
 Std. Pressure (mm Hg): 760
 K₁ (K/mm Hg): 0.3857

Reference Equipment

WTM Model: W-NKoDa-5B WTM Cal. Due Date: Dec. 2024
 WTM Serial: 600245 Gamma: 1.0000

UUT Meter (DGM)					Reference Meter (WTM)				
Run Time (minutes)	DGM Orifice (mm H ₂ O)	Volume		Outlet Temp		Volume		Outlet Temp	
		Initial	Final	Initial	Final	Initial	Final	Initial	Final
0	P _{m(ga)}	V _{mz}	V _{mf}	t _m	t _{mf}	V _w	V _{wf}	t _w	t _{wf}
15.00	13.0	107.7550	107.9221	29	30	68.41024	68.57350	28	27
10.00	25.0	107.9308	108.0876	30	30	68.58202	68.73488	27	27
8.00	50.0	108.1027	108.2822	30	30	68.74958	68.92516	27	27
7.00	80.0	108.3029	108.5061	30	30	68.94550	69.14488	27	27
5.00	120.0	108.5139	108.6908	30	30	69.15251	69.32550	27	27

Standardized Data

Test Meter		Reference Meter		Correction Factor		Calibration Results		
Std. Volume	Std. Flow Rate	Std. Volume	Std. Flow Rate	"Gamma"	Variation	Flow Rate	ΔH@ (mm H ₂ O)	Variation
V _{test} (m ³)	Q _{test} m ³ /min	V _{ref} (m ³)	Q _{ref} m ³ /min	(Y)	(ΔY)	Q _{test/corr}	0.0212 SCMM	ΔH _{sc}
0.162	0.011	0.159	0.011	0.982	0.000	0.011	50.751	2.535
0.152	0.015	0.149	0.015	0.982	0.001	0.015	49.300	1.084
0.174	0.022	0.171	0.021	0.983	0.002	0.021	48.061	-0.155
0.197	0.028	0.194	0.028	0.983	0.002	0.028	45.922	-2.293
0.173	0.035	0.169	0.034	0.976	-0.005	0.034	47.046	-1.170
				0.981	= Y Avg	48.216 = ΔH@ Avg		

Pass/Fail Result: **Pass**

Note: For Calibration Factor Y, the ratio of the reading of the calibration meter to the dry gas meter, acceptable tolerance of individual values from the average is ±0.02

Note: For ΔH_{sc}, orifice pressure differential that equates to 0.75cfm (0.0212m³/min) at standard temperature and pressure, acceptable tolerance of individual values from the average is ±0.2inches (5.1mm) H₂O

Approved By: _____

(Patpasu Chaisana)
 Service Manager

WISDOM SCIENCE
 บริษัท วิสโดม ไซนส์ แอนด์ เซอร์วิส กรุ๊ป จำกัด
 WISDOM SCIENCE SALE AND SERVICE GROUP COMPANY LIMITED

Date: 04-Aug-24

COPY

Certificate of Calibration - Supplemental

METHOD 5 PRE-TEST CONSOLE CALIBRATION

Nomenclature

P_b - Barometric Pressure
 DGM - Dry Gas Meter
 K₁ - Constant based on standard temp and press
 t - Run time, in minutes
 P_m - ΔH (Meter Pressure, gauge)
 V_m - Volume collected by test meter, corrected for STP
 Q_{m(test)} - Calculated flow rate of test meter
 K' - Critical orifice coefficient
 P_w - Measured pressure of reference meter
 t_w - Temperature measured in reference meter
 t_m - Temperature measured in test meter
 Y - Ratio of volume collected from test meter and orifice
 sc - Scaling Factor
 Counts_{sc} - Number of pulse counts, standardized
 Counts_{total} - Number of raw pulse counts of a calibration run

Equations

$$V_{m(std)} = Y * K_1 \frac{P_w * (P_{bar} + \frac{P_m}{1.3})}{T_w}$$

$$V_{m(std)} = Counts_{std} * Y_{sc(avg)}$$

$$Counts_{std} = K_1 \frac{Counts_{total} * (P_{bar} + \frac{P_m}{1.3})}{T_w}$$

$$Q_{m(std)} = \frac{V_{m(std)}}{t}$$

$$Y_{sc} = \frac{V_{m(std)}}{Counts_{std}}$$


$$K_1 = \frac{T_{std}}{P_{std}}$$

$$Y = \frac{V_{m(std)}}{V_{ref}}$$

$$Y_{sc} = \frac{Counts_{std}}{Counts_{total}}$$


$$Y_{sc} = \frac{P_{std}}{P_{std} + \frac{P_m}{1.3}} * \left(\frac{T_{std}}{T_w} \right)$$

Calibration Train

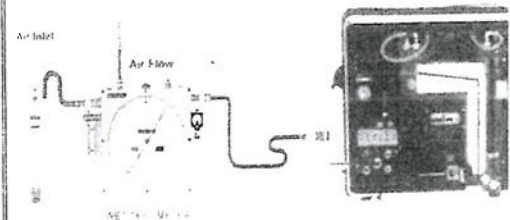

Calibration Graphs


Meter Pressure vs Flowrate

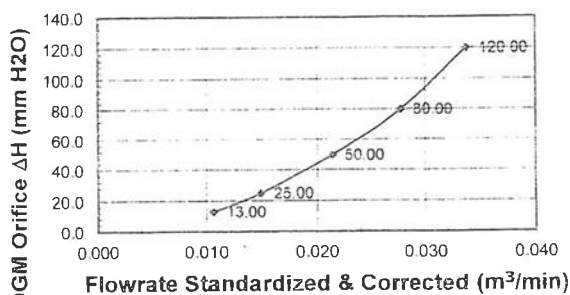

Console Serial: 1007055

Console Model: MC-

Meter Gamma vs Flowrate

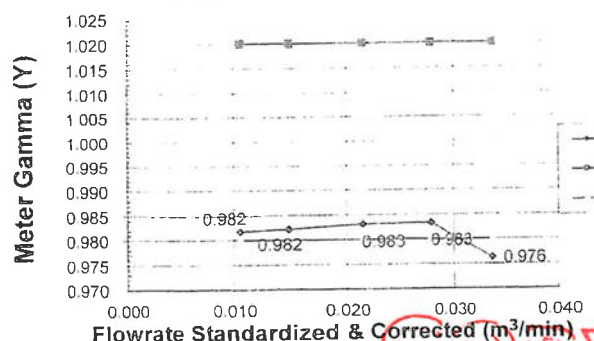

Console Serial: 1007055

Console Model: MC-572-V



WISDOM SCIENCE

TEMPERATURE DISPLAY CALIBRATION

Meter Console Information

Console Model	MC-572-V
Console serial	1007055
Temp Indicator Model	765-KF
Temp Indicator Serial	JC17852

Calibration Conditions

Cal Date	04-Aug-24
Due Date	04-Aug-25
Cal Report No	WDS-SV8707001
Ambient Temp (°C)	25
Pressure (mm Hg)	758
Humidity (%)	60

Reference Equipment

Temp Meter Model	Fuke 7-48
Serial No	60590035
Cal Date	07-Apr-24
Temp Meter Model	Fuke 179
Serial No	59620112
Cal Date	06-Feb-24

Temperature Sensor Calibration

Reference Point #	Ref Thermometer Temperature °C	Thermocouple Display Temperature °C	Temperature Difference °C
1	-18.0	-18.0	0.0
2	38.0	38.0	0.0
3	93.0	94.0	-1.0
4	149.0	149.0	0.0
5	260.0	261.0	-1.0
6	371.0	372.0	-1.0
7	482.0	482.0	0.0
8	593.0	593.0	0.0
9	816.0	816.0	0.0
10	1038.0	1038.0	0.0
Maximum ¹			1.0

Note

¹ For valid test results, the maximum difference between temperature readings should $\leq 1.0^\circ\text{C}$ (EPA Method 5, Section 6.1.1.8). Perform all TC Channel calibrations. Except meter (DGM) channel

PASS

DGM Out Temperature Sensor Calibration

Temperature point #	Ref Thermometer Temperature °C	Thermocouple Display Temperature °C	Temperature Difference °C
Ice	0.0	0.0	0.0
Ambient	28.9	27.0	-0.1
Heat	114.5	115.0	-0.5
Difference Rang			
Temp. Difference	$\pm 2^\circ\text{F}$ or $\pm 1.1^\circ\text{C}$		

PASS

Note

The temperatures of the thermocouple and reference thermometers shall agree to within $\pm 2^\circ\text{F}$ (EPA Method 5, section 10.5)

Approved By :

Patpasu Chaisana

(Patpasu Chaisana)

Service Manager

WISDOM SCIENCE

บริษัท วิสโดม ไซนซ์ จำกัด

WISDOM SCIENCE SALE AND SERVICE GROUP COMPANY LIMITED

COPY



Calibration Certificate

ENTECH
Difference For Greater Value

Certificate No: G 670415
Date of issue : 25-Jun-24

Instrument description : Flue Gas Analyzer
Instrument model : Testo 350XL
Control unit serial no. : 01794619/002
Instrument serial no. : 01807527/002
ID no. or control no. : -
Manufacturer : Testo SE & Co. KGaA
Probe description : -
Probe model : -
Probe serial no. : -
Customer name : Eastern Thal Consulting 1992 Company Limited
Customer address : 683 Moo 11, Sukhapibarn 8 Road, Nongkham, Si Racha, Chon Buri 20280

Total pages of certificate : 2 Pages
Receiving no. : L-242269
Receiving date. : 19-Jun-24
Parameter of calibration : Gas Calibration(Oxygen 2.50,10.04,21.02 %vol, Carbon Monoxide 80.18,302,1001 ppm, Nitrogen Dioxide 30.34,81.32, 201.9 ppm, Nitric Oxide 30.01, 151.5, 322.5 ppm, Sulphur Dioxide 50.36, 100.8, 600.8 ppm)
Condition of UUC. : Used
Ambient condition : All of the Measurement were carried out the stabilized laboratory

Temperature : 23 ±5 °C
Humidity : 55 ± 15 %RH
Calibration place : 17/121 Soi Ngamwongwan 47 Yaek 48, Toongsonghong, Laksi, Bangkok 10210
Calibration procedure no. : This instrument was calibrated by comparison with Standard gas mixture according to calibration Work Instruction no. WI-CL-28-C

The calibration certificate expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%. This certificate is applied only to item under test Environmental condition.
This Calibration Certificate may not be reproduced other than in full except with the permission of the issuing laboratory. Calibration certificates without signature and seal not valid and The results relate only to the items tested/calibrated.
This calibration certificate documents are traceability to national standards, which realize measurement according to the International System of Units (SI).

Date of calibration : 24-Jun-24

Kwanchoi K.

Mr. Kwanchai Khamdoun
Calibration Technician

9098 9098

Mr. Nongnuch Hariraila
Technical Manager



Calibration Certificate

Certificate No.: G 670415

Standard References (Table 1)

Standard	Certificate No.	Vendor	Due date
Oxygen (O2) 2.50 % Vol	2412/23	Linde	27-Aug-27
Oxygen (O2) 10.04 % Vol	CG-0153-21	Nimt	18-Nov-26
Oxygen (O2) 21.02 % Vol	CG-0041-22	Nimt	10-Feb-27
Carbon monoxide (CO) 80.18 ppm	CG-0002-24	Nimt	11-Jan-29
Carbon monoxide (CO) 302 ppm	1915/23	Linde	16-Jun-25
Carbon monoxide (CO) 1001 ppm	CG-0085-24	Nimt	22-May-29
Nitrogen Dioxide (NO2) 30.34 ppm	2703/22	Linde	22-Aug-24
Nitrogen Dioxide (NO2) 81.32 ppm	3546/23	Linde	14-Jan-26
Nitrogen Dioxide (NO2) 201.9 ppm	1975/23	Linde	17-Jul-25
Nitric Oxide (NO) 30.01 ppm	CG-0014-23	Nimt	19-Feb-25
Nitric Oxide (NO) 151.5 ppm	0161/23	Linde	22-Jan-25
Nitric Oxide (NO) 322.5 ppm	1974/23	Linde	17-Jul-25
Sulphur Dioxide (SO2) 50.36 ppm	2004/23	Linde	17-Jul-25
Sulphur Dioxide (SO2) 100.8 ppm	3507/22	Linde	09-Nov-24
Sulphur Dioxide (SO2) 600.8 ppm	2003/23	Linde	17-Jul-25

Measured room conditions

Temperature : 24.1 °C Humidity : 62.8 %RH Pressure : 1009.9 mbar

Calibration conditions

Gas Temperature : 24 °C Flow rate : 1,000 ml/min Gas pressure : 1014.7 mbar

Calibration Results (Without adjustment) (Table 2)

Parameter of Standard	Standard Values	Mean of UUC	Error	Uncertainty (±)
O2 (%Vol)	2.50	2.48	-0.02	0.15
O2 (%Vol)	10.04	9.93	-0.11	0.20
O2 (%Vol)	21.02	21.11	0.09	0.30
CO (ppm)	80.18	81	0.82	3.0
CO (ppm)	302	302	0	6.0
CO (ppm)	1001	1002	1	12
NO2 (ppm)	30.34	31.5	1.16	8.0
NO2 (ppm)	81.32	82.3	0.98	8.0
NO2 (ppm)	201.9	201.2	-0.7	12
NO (ppm)	30.01	32	1.99	8.0
NO (ppm)	151.5	155	3.5	8.0
NO (ppm)	322.5	327	4.5	12
SO2 (ppm)	50.36	49	-1.36	6.0
SO2 (ppm)	100.8	100	-0.8	6.0
SO2 (ppm)	600.8	602	1.2	13

Remark : 1 cmol/mol = 1 %vol. 1 μmol/mol = 1 ppm.

End of Report





CERTIFICATE OF CALIBRATION

Page 1 of 3

Certificate No. : 23-148804
Sample Code : 23-56200-006

Customer : EASTERN THAI CONSULTING 1992 CO., LTD.

683 Moo 11, Sukhapibarn 8 Rd., Nongkham,

Sriracha, Chonburi 20230

Location of Calibration : EASTERN THAI CONSULTING 1992 CO., LTD.

(Hot Lab)

Equipment : Temperature controlled enclosures (Hot air oven)

Manufacturer : Mammert Model : UFE 500

Serial No. : G511.0182 ID No. : LABE 17/4

Date of Receipt : 22 December 2023 Date of Calibration : 22 December 2023

Condition of Calibration

1. Environment	1.1 Ambient temperature	: Maximum	30.9 °C	: Minimum	29.6 °C
	1.2 Relative humidity	: Maximum	54.5 %	: Minimum	46.8 %
	1.3 Line voltage supplied	: Maximum	227.6 VAC	: Minimum	224.2 VAC

2. Calibration method

TLAS-G-20: Guidelines for calibration and checks of temperature controlled enclosures.

3. Reference standard instrument

Instrument	ID No.	Certificate No.	Due Date
Data Acquisition With Sensor (RTD-PT100)	LB-DA-08 (RTD-248 to RTD-256)	23-084070	06 August 2024

4. This certificate is traceable to the international system of unit (SI Unit).

The measurement is traceable to Asia Medical and Agricultural Laboratory and Research Center Public Company Limited.

5. This result of calibration was found accurate as shown on date and place of calibration only.

6. Condition of calibration item : Normal

Calibrated by

Mr. Risak Into

(Mr. Somchai Neampunt)

Scientist

Signed for Director

Issue date

25 December 2023

The uncertainties are for a confidence probability of approximately 95%.

The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognised national standards and to the unit of measurement realised at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Asia Medical and Agricultural Laboratory and Research Center Public Company Limited (AMARC)

361 Soi Ladprao 122, Ladprao Road,

Phlabapha, Wang Thonglang, Bangkok 10310

Rev 01

TEL 02-516-2422

FAX 02-516-6949

Rev 01

CONTACT@AMARC.CO.TH

WWW.AMARC.CO.TH

Effective Date 15/10/21



REPORT OF CALIBRATION

Page 2 of 3

Certificate No. : 23-148804
Sample Code : 23-56200-006

Results of Calibration

Resolution : 0.5 °C

1. Reporting of Temperature

Calibration point (°C)	UUC* setting (°C)	UUC* reading (°C)	Measured temperature at each positions (°C)								Uncertainty ± (°C)	Coverage factor k	
			# 1	# 2	# 3	# 4	# 5	# 6	# 7	# 8			# 9 ^{ref}
104	103.5	103.5	104.11	103.94	103.85	103.84	103.97	103.93	103.64	103.51	104.23	0.47	2.00

2. Characterization results

Calibration point (°C)	Stability ± (°C)	Uniformity (°C)	Overall variation (°C)
104	0.04	0.78	0.81

Notes

UUC* = Unit Under Calibration

COPY

361 Soi Ladprao 122, Ladprao Road,

Phlabapha, Wang Thonglang, Bangkok 10310

Rev 08

TEL 02-516-2422

FAX 02-516-6949

Rev 08

CONTACT@AMARC.CO.TH

WWW.AMARC.CO.TH

Effective Date 15/10/21



REPORT OF CALIBRATION


Certificate No. : 23-148804

Sample Code : 23-56200-006

Results of Calibration

Notes

1. Sensor installation locations
 - 1.1 All sensors at any corners or walls should be positioned 5 cm (a x b x c) from the wall.
 - 1.2 The reference sensor is preferably located of the geometric center of the chamber.
2. Interior dimensions approx of chamber :
W = 56 cm ; D = 40 cm ; H = 48 cm
3. Air valve or fresh air level : Off
4. Fan level : Open
5. The quoted uncertainty includes "Stability of chamber and loading effect in chamber at 20% of uniformity".
6. Uniformity - the maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time.
7. Stability - one-half of the greatest maximum difference of measured temperatures at any one sensor.
8. Overall variation - the difference of the maximum and the minimum measured temperatures throughout observation time.
9. UUC* reading - the average reading of indicating device that forms the integral part of the enclosure.
10. Calibration results without adjustment.

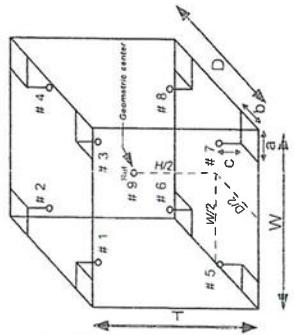Figure: Example of sensor
Installation Positions

The result expanded uncertainty of measurement U is stated as the standard uncertainty of measurement multiplied by the coverage factor k, which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty of measurement has been determined in accordance with UKAS M3003.

- End of Report -

COPY



Bara Scientific Co., Ltd.
988 U Chu Liang Building Floor7 Rama4 Road
Silom Bangkok Bangkok Thailand 10500
Tel : 02-6324300 Fax : 02-6375496-7
www.barascientific.com



Certificate of Calibration

Number of Page(s) 1 of 3

Certificate No.

BSCC-UV-146/24

Equipment

UV/Vis Spectrophotometer

Model

UV-1800

Manufacturer

Shimadzu

Serial No.

A11635101643 CD

ID No.

LABE 03/2

Date of receipt

22 April 2024

Date of calibration

22 April 2024

Date of issue

29 April 2024

Customer name

Eastern Thai Consulting 1992 Co., Ltd.

Address

683 Moo 11, Sukkaphitbarn 8 Rd., Nongkham, Sriracha, Chonburi 20230

Temperature

(22.9-24.1) °C (On site)

Humidity

(41.7-46.9) %RH (On site)

Equipment condition

Good Operation

Calibration Location

Analysis Department

Calibration Procedure

In-house method WI-UV-702-01 based on ASTM E275-01

Traceability

Wavelength Accuracy is traceable to certificate No. 116614 and 116613

Photometric Accuracy is traceable to certificate No. 116210 and 116224

Siray Light is traceable to certificate No. 116616

The above certificate are traceable to SI unit through Siama Scientific Ltd.

(UKAS accredited calibration laboratory NO. 0659)

Calibrated by

Mr. Poomjai Korsawatvorakul

Approved by

Mr. Sonthi Temboonsakdi
Service Manager

The above results are valid exclusively for the calibrated item(s) as mention in this report / certificate
Advertising the report / Certificate and publicity of the results are prohibited and also shall not be reproduced
except in full, without written approval of the Bara Scientific Co., Ltd.

COPY



Bara Scientific Co., Ltd.
988 U Chu Liang Building Floor7 Rama4 Road
Silom Bangkok Bangkok Thailand 10500
Tel : 02-6324300 Fax : 02-6375496-7
www.barascientific.com



Certificate of Calibration

Certificate No.

BSCC-UV-146/24

Calibration Results:

1. Wavelength Accuracy

Certified Wavelength (nm)	UUC (nm)	Error (nm)	Uncertainty (±nm)
287.71	287.75	0.04	0.18
445.82	445.89	0.07	0.18
536.52	536.50	-0.02	0.18
741.02	741.01	-0.01	0.18
879.41	879.33	-0.08	0.18

2. Photometric Accuracy (UV)

Wavelength (nm)	Certified Absorbance (A)	UUC (A)	Error (A)	Uncertainty (±A)
235	0.0000	0.0000	0.0000	0.0075
	0.7415	0.7387	-0.0028	0.0075
257	CNR	CNR	CNR	CNR
	CNR	CNR	CNR	CNR
313	CNR	CNR	CNR	CNR
	CNR	CNR	CNR	CNR
350	0.0000	0.0000	0.0000	0.0075
	0.6406	0.6395	-0.0011	0.0075

*CNR = Customer not request

The above results are valid exclusively for the calibrated item(s) as mention in this report / certificate
Advertising the report / Certificate and publicity of the results are prohibited and also shall not be reproduced
except in full, without written approval of the Bara Scientific Co., Ltd.



Bara Scientific
Sole agent of Success
Bara Scientific Co., Ltd.
968 U Chu Liang Building Floor 7 Rama4 Road
Silom Bangkok Thailand 10500
Tel : 02-6324300 Fax : 02-6376486-7
www.barascientific.com



Certificate of Calibration

Certificate No. BSCC-UV-146/24 Number of Page(s) 3 of 3

Calibration Results:

3. Photometric Accuracy (Visible)

Wavelength (nm)	Certified Absorbance (A)	UUC (A)	Error (A)	Uncertainty (±A)
420.0	0.0000	0.0000	0.0000	0.0042
	0.5715	0.5729	0.0014	0.0042
	0.7087	0.7087	0.0000	0.0042
440.0	1.0987	1.1005	0.0018	0.0042
	0.0000	0.0000	0.0000	0.0042
	0.5561	0.5578	0.0017	0.0042
	0.6968	0.6969	0.0001	0.0042
	1.0757	1.0774	0.0017	0.0042
465.0	CNR	CNR	CNR	CNR
	CNR	CNR	CNR	CNR
	CNR	CNR	CNR	CNR
546.1	0.0000	0.0000	0.0000	0.0042
	0.5193	0.5213	0.0020	0.0042
	0.6937	0.6940	0.0003	0.0042
	1.0411	1.0428	0.0017	0.0042
590.0	CNR	CNR	CNR	CNR
	CNR	CNR	CNR	CNR
	CNR	CNR	CNR	CNR
635.0	0.0000	0.0000	0.0000	0.0042
	0.5605	0.5624	0.0019	0.0042
	0.7579	0.7583	0.0004	0.0042
	1.1131	1.1138	0.0007	0.0042

*CNR = Customer not request

4. Stray Light*

Standard cut-off wavelength (nm)	Unit Under Calibration(UUC)	
	Wavelength (nm)	Absorbance (A)
201.33±0.11nm	200.80	2.0111

The Stray light transmission reference is less than 1.0%T and Stray light absorbance reference is greater than 2.00A
*Stray Light not NSC-ONSC Accredited.

The measurement uncertainty is base on a standard uncertainty multiplied by a coverage factor k=2 providing a level of confidence of approximately 95%

End of Certificate

The above results are valid exclusively for the calibrated item(s) as mention in this report / certificate
Advertising the report / Certificate and publicity of the results are prohibited and also shall not be reproduced except in full, without written approval of the Bara Scientific Co., Ltd

COPY



CALIBRATION CERTIFICATE

Certificate No. : L202406089-0003

Date Issued : 12-Jun-24

Customer : Eastern Thai Consulting 1992 Co., Ltd.
683 Moo 11, Sukhapibarn 8 Rd., Nongkham, Sriracha, Chonburi 20230

Equipment : Area Heat Stress Monitor

Manufacturer : TSI

Model : QUESTEMP 34

Serial No. : TEU080013

ID No./Tag No. : NO.12

Date Received : 10-Jun-24

Date Calibrated : 10-Jun-24

Calibrated by : Apiwat Peanrungronth

Calibration Method or Calibration Procedure Used


In-house method : CP-19 by comparing against Standard Digital Humidity / Temperature Meter

This certificate is traceable to national standards, which realize the units of measurement according to the International System of Units (SI).

Result of Calibration

The reported uncertainty of measurement was based on standard uncertainty multiplied by a coverage factor $k = 2$, providing a level confidence approximately 95 percent.

This certificate may not be reproduced other than in full except with the prior written approval of the Miracle International Technology Company Limited.

Approved by: 
(Sarayuth Tochua)



Page 1 of 2

COPY

Certificate No. : L202406089-0003

Environment : Ambient Temperature : (25 ± 2) °C

Relative Humidity : (50 ± 15)%RH

STD	UUC Reading (°C)	UUC Error	Measurement	MPE	Pass / Fail
Reading (°C)	Before Adjusted	After Adjusted	Uncertainty (±°C)	(±°C)	Simple Acceptance
38.00	WET 37.8	-	0.35	0.5	Pass
38.00	DRY 38.0	-	0.35	0.5	Pass
38.00	GLOBE 37.7	-	0.35	0.5	Pass
44.99	WET 44.9	-	0.35	0.5	Pass
44.99	DRY 45.2	-	0.35	0.5	Pass
44.99	GLOBE 44.8	-	0.35	0.5	Pass

STD = Standard

Pass = |error| ≤ |MPE|

UUC = Unit Under Calibration

Fail = |error| > |MPE|

Description of UUC :

Range

0 to 100 °C

Resolution

0.1 °C

Condition As-Received : Used Item

The measurement results and statements of conformity with specification only relate to the item calibrated.

Measurement Standards Used & Traceability :

The International System of Units (SI) through

MIT Certificate No. L202310317-0003 for Digital Thermometer with Probe (Fluke) Serial No. 5856603, Due 06-Nov-24

End of Certificate

Page 2 of 2

COPY



MIRACLE INTERNATIONAL TECHNOLOGY CO.,LTD
214 Bangwaek Rd. Bangpai Bangkok 10160
Tel : 0-2865-4647-8 Fax: 0-2865-4649 <http://www.mti.in.th>



CALIBRATION CERTIFICATE

Certificate No. : L202406089-0001

Date Issued : 12-Jun-24

Customer : Eastern Thai Consulting 1992 Co., Ltd.
683 Moo 11, Sukhapibam 8 Rd., Nongkham, Sriracha, Chonburi 20230

Equipment : Area Heat Stress Monitor

Manufacturer : TSI
Model : QUESTEMP 34
Serial No. : TEU080011
ID No./Tag No. : NO.10
Date Received : 10-Jun-24
Date Calibrated : 10-Jun-24
Calibrated by : Apiwat Peanrungronth

Calibration Method or Calibration Procedure Used


In-house method : CP-19 by comparing against Standard Digital Humidity / Temperature Meter

This certificate is traceable to national standards, which realize the units of measurement according to the International System of Units (SI).

Result of Calibration

The reported uncertainty of measurement was based on standard uncertainty multiplied by a coverage factor $k = 2$, providing a level confidence approximately 95 percent.

This certificate may not be reproduced other than in full except with the prior written approval of the Miracle International Technology Company Limited.



Approved by: *Sarayuht T.*
(Sarayuht Tochua)

Page 1 of 2

COPY

Certificate No. : L202406089-0001

Environment : Ambient Temperature : $(25 \pm 2) ^\circ\text{C}$

Relative Humidity : $(50 \pm 15)\%\text{RH}$

STD	UUC Reading (°C)		UUC Error	Measurement	MPE	Pass / Fail
Reading (°C)	Before Adjusted	After Adjusted	(°C)	Uncertainty (±°C)	(±°C)	Simple Acceptance
38.00	WET 38.1	-	0.10	0.35	0.5	Pass
38.00	DRY 37.8	-	-0.20	0.35	0.5	Pass
38.00	GLOBE 38.2	-	0.20	0.35	0.5	Pass
44.99	WET 44.9	-	-0.09	0.35	0.5	Pass
44.99	DRY 44.7	-	-0.29	0.35	0.5	Pass
44.99	GLOBE 45.1	-	0.11	0.35	0.5	Pass

STD = Standard

Pass = $|\text{error}| \leq |\text{MPE}|$

UUC = Unit Under Calibration

Fail = $|\text{error}| > |\text{MPE}|$

Description of UUC : Range 0 to 100 $^\circ\text{C}$

Resolution 0.1 $^\circ\text{C}$

Condition As-Received : Used Item

The measurement results and statements of conformity with specification only relate to the item calibrated.

Measurement Standards Used & Traceability :

The International System of Units (SI) through

MIT Certificate No. L202310317-0003 for Digital Thermometer with Probe (Fluke) Serial No. 5856603, Due 06-Nov-24

End of Certificate

Page 2 of 2

COPY



MIRACLE INTERNATIONAL TECHNOLOGY CO., LTD
214 Bangwek Rd. Bangpai Bangkok 10160
Tel.: 0-2865-4647-8 Fax: 0-2865-4649 <http://www.mit.in.th>



CALIBRATION CERTIFICATE

Customer

: Eastern Thai Consulting 1992 Co., Ltd.
683 Moo 11, Sukhaphibarn 8 Rd., Nongkham, Sriracha, Chonburi 20230

Equipment

: Area Heat Stress Monitor

Manufacturer

: TSI

Model

: QUESTEMP 34

Serial No.

: TEU080014

ID No./Tag No.

: NO.13

Date Received

: 28-Jun-24

Date Calibrated

: 28-Jun-24

Calibrated by

: Apiwat Peanrungrath

Calibration Method or Calibration Procedure Used

In-house method : CP-19 by comparing against Standard Digital Humidity / Temperature Meter

This certificate is traceable to national standards, which realize the units of measurement according to the International System of Units (SI).

Result of Calibration

The reported uncertainty of measurement was based on standard uncertainty multiplied by a coverage factor $k = 2$, providing a level confidence approximately 95 percent.

This certificate may not be reproduced other than in full except with the prior written approval of the Miracle International Technology Company Limited.

Approved by:

Sorayuth T.
(Sarayuth Tochua)



Page 1 of 2

COPY

Certificate No. :

L202406394-0001

Environment :

Ambient Temperature :
(25 ± 2) °C

Relative Humidity :

(50 ± 15)%RH

STD	UUC Reading (°C)	UUC Error (°C)	Measurement	MPE (±°C)	Pass / Fail
Reading (°C)	Before Adjusted	After Adjusted	Uncertainty (±°C)		Simple Acceptance
37.98	WET 38.0	-	0.35	0.5	Pass
37.98	DRY 38.0	-	0.35	0.5	Pass
37.98	GLOBE 38.0	-	0.35	0.5	Pass
44.99	WET 45.0	-	0.35	0.5	Pass
44.99	DRY 44.9	-	0.35	0.5	Pass
44.99	GLOBE 45.0	-	0.35	0.5	Pass

STD = Standard

Pass = $|\text{error}| \leq |\text{MPE}|$

UUC = Unit Under Calibration

Fail = $|\text{error}| > |\text{MPE}|$

Description of UUC :

Range 0 to 100 °C

Resolution

0.1 °C

Condition As-Received : Used Item

The measurement results and statements of conformity with specification only relate to the item calibrated.

Measurement Standards Used & Traceability :

The International System of Units (SI) through

MIT Certificate No. L202310317-0003 for Digital Thermometer with Probe (Fluke) Serial No. 5856603, Due 06-Nov-24

End of Certificate

Page 2 of 2

COPY



MIRACLE INTERNATIONAL TECHNOLOGY CO.,LTD
214 Bangpak Rd. Bangpai, Bangkok 10160
Tel.: 0-2865-4647-8 Fax: 0-2865-4649 <http://www.mit.in.th>



CALIBRATION CERTIFICATE

Customer

: Eastern Thai Consulting 1992 Co., Ltd.
683 Moo 11, Sukhapibam 8 Rd., Nongkham, Sriracha, Chonburi 20230

Equipment

: Area Heat Stress Monitor

Manufacturer

: TSI

Model

: QUESTEMP 34

Serial No.

: TEU080012

ID No./Tag No.

: NO.11

Date Received

: 10-Jun-24

Date Calibrated

: 10-Jun-24

Calibrated by

: Apiwat Peanrungrath

Calibration Method or Calibration Procedure Used

In-house method : CP-19 by comparing against Standard Digital Humidity / Temperature Meter

This certificate is traceable to national standards, which realize the units of measurement according to the International System of Units (SI).

Result of Calibration

The reported uncertainty of measurement was based on standard uncertainty multiplied by a coverage factor $k = 2$, providing a level confidence approximately 95 percent.

This certificate may not be reproduced other than in full except with the prior written approval of the Miracle International Technology Company Limited.

Approved by:

Sorayuth T.
(Sorayuth Tochua)

Page 1 of 2

COPY

Certificate No. : L202406089-0002

Environment :

Ambient Temperature :

(25 ± 2) °C

Relative Humidity :

(50 ± 15)%RH

STD	Reading (°C)	Before Adjusted	After Adjusted	UUC Error (°C)	Measurement	MPE (±°C)	Pass / Fail
38.00	WET	38.0	-	0.00	0.35	0.5	Pass
38.00	DRY	37.8	-	-0.20	0.35	0.5	Pass
38.00	GLOBE	37.9	-	-0.10	0.35	0.5	Pass
44.99	WET	45.2	-	0.21	0.35	0.5	Pass
44.99	DRY	45.0	-	0.01	0.35	0.5	Pass
44.99	GLOBE	44.9	-	-0.09	0.35	0.5	Pass

STD = Standard

UUC = Unit Under Calibration

Pass = $|\text{error}| \leq |\text{MPE}|$

Fail = $|\text{error}| > |\text{MPE}|$

Description of UUC :

Range

0 to 100 °C

Resolution

0.1 °C

Condition As-Received : Used Item

The measurement results and statements of conformity with specification only relate to the item calibrated.

Measurement Standards Used & Traceability :

The International System of Units (SI) through

MIT Certificate No. L202310317-0003 for Digital Thermometer with Probe (Fluke) Serial No. 5856603, Due 06-Nov-24

End of Certificate

Page 2 of 2

COPY



MIRACLE INTERNATIONAL TECHNOLOGY CO.,LTD
214 Bangwaek Rd. Bangpai Bangkok 10160
Tel.: 0-2865-4647-8 Fax: 0-2865-4649 <http://www.mit.in.th>



CALIBRATION CERTIFICATE

Certificate No. : L202406394-0001
Date Issued : 01-Jul-24

Customer : Eastern Thai Consulting 1992 Co., Ltd.
683 Moo 11, Sukhapibarn 8 Rd., Nongkharn, Sriracha, Chonburi 20230

Equipment : Area Heat Stress Monitor

Manufacturer : TSI

Model : QUESTEMP 34

Serial No. : TEU080014

ID No./Tag No. : NO.13

Date Received : 28-Jun-24

Date Calibrated : 28-Jun-24

Calibrated by : Apiwat Peanrungrath

Calibration Method or Calibration Procedure Used

In-house method : CP-19 by comparing against Standard Digital Humidity / Temperature Meter

This certificate is traceable to national standards, which realize the units of measurement according to the International System of Units (SI).

Result of Calibration

The reported uncertainty of measurement was based on standard uncertainty multiplied by a coverage factor $k = 2$, providing a level confidence approximately 95 percent.

This certificate may not be reproduced other than in full except with the prior written approval of the Miracle International Technology Company Limited.

Approved by:

Saranyuth T.
(Saranyuth Tochua)



Page 1 of 2

COPY

Certificate No. : L202406394-0001

Environment : Ambient Temperature : $(25 \pm 2) ^\circ\text{C}$

Relative Humidity : $(50 \pm 15)\%\text{RH}$

STD	UUC Reading ($^\circ\text{C}$)	UUC Error ($^\circ\text{C}$)	Measurement	MPE ($\pm^\circ\text{C}$)	Pass / Fail
Reading ($^\circ\text{C}$)	Before Adjusted	After Adjusted	Uncertainty ($\pm^\circ\text{C}$)		Simple Acceptance
37.98	WET 38.0	-	0.35	0.5	Pass
37.98	DRY 38.0	-	0.35	0.5	Pass
37.98	GLOBE 38.0	-	0.35	0.5	Pass
44.99	WET 45.0	-	0.35	0.5	Pass
44.99	DRY 44.9	-	0.35	0.5	Pass
44.99	GLOBE 45.0	-	0.35	0.5	Pass

STD = Standard

Pass = $|\text{error}| \leq |\text{MPE}|$

UUC = Unit Under Calibration

Fail = $|\text{error}| > |\text{MPE}|$

Description of UUC :

Range

0 to 100 $^\circ\text{C}$

Resolution

0.1 $^\circ\text{C}$

Condition As-Received : Used Item

The measurement results and statements of conformity with specification only relate to the item calibrated.

Measurement Standards Used & Traceability :

The International System of Units (SI) through

MIT Certificate No. L202310317-0003 for Digital Thermometer with Probe (Fluke) Serial No. 5856603, Due 06-Nov-24

End of Certificate

Page 2 of 2

COPY



MIRACLE INTERNATIONAL TECHNOLOGY CO.,LTD
214 Bangwek Rd. Bangpai Banglae Bangkok 10160
Tel.: 0-2863-4647-8 Fax: 0-2863-4649 <http://www.mit.in.th>



CALIBRATION CERTIFICATE

Certificate No. : L202406394-0003

Date Issued : 01-Jul-24

Customer
: Eastern Thai Consulting 1992 Co., Ltd.
683 Moo 11, Sukhapibarn 8 Rd., Nongkham, Sriracha, Chonburi 20230

Equipment
: Area Heat Stress Monitor

Manufacturer
: TSI
Model
: QUESTEMP 34

Serial No.
: TEU080015

ID No./Tag No.
: NO.14

Date Received
: 28-Jun-24

Date Calibrated
: 28-Jun-24

Calibrated by
: Apiwat Peanrungrath

Calibration Method or Calibration Procedure Used

In-house method : CP-19 by comparing against Standard Digital Humidity / Temperature Meter

This certificate is traceable to national standards, which realize the units of measurement according to the International System of Units (SI).

Result of Calibration

The reported uncertainty of measurement was based on standard uncertainty multiplied by a coverage factor $k = 2$, providing a level confidence approximately 95 percent.

This certificate may not be reproduced other than in full except with the prior written approval of the Miracle International Technology Company Limited.

Approved by:

Sorayuth T.
(Sorayuth Tochua)



Page 1 of 2

COPY

Certificate No. : L202406394-0003

Environment : Ambient Temperature : $(25 \pm 2) ^\circ\text{C}$

Relative Humidity : $(50 \pm 15)\%\text{RH}$

STD Reading ($^\circ\text{C}$)	Before Adjusted	After Adjusted	UUC Error ($^\circ\text{C}$)	Measurement Uncertainty ($\pm^\circ\text{C}$)	MPE ($\pm^\circ\text{C}$)	Pass / Fail Simple Acceptance
37.98	WET 38.1	-	0.12	0.35	0.5	Pass
37.98	DRY 38.2	-	0.22	0.35	0.5	Pass
37.98	GLOBE 37.8	-	-0.18	0.35	0.5	Pass
44.99	WET 45.1	-	0.11	0.35	0.5	Pass
44.99	DRY 45.2	-	0.21	0.35	0.5	Pass
44.99	GLOBE 44.8	-	-0.19	0.35	0.5	Pass

STD = Standard

Pass = $|\text{error}| \leq |\text{MPE}|$

UUC = Unit Under Calibration

Fail = $|\text{error}| > |\text{MPE}|$

Description of UUC :

Range

0 to 100 $^\circ\text{C}$

Resolution

0.1 $^\circ\text{C}$

Condition As-Received : Used Item

The measurement results and statements of conformity with specification only relate to the item calibrated.

Measurement Standards Used & Traceability :

The International System of Units (SI) through

MIT Certificate No. L202310317-0003 for Digital Thermometer with Probe (Fluke) Serial No. 5856603, Due 06-Nov-24

End of Certificate

Page 2 of 2

COPY

Cert. No. : ACC24014
Pages : 1 of 3

Cert. No. : ACC24014
Job No. : VC67AC0083
Pages : 2 of 3

Calibration Certificate

Equipment : SOUND CALIBRATOR
Manufacturer : RION
Model : NC-75
Serial No.: 34302326
ID No.:

Condition As Found : GOOD

Customer : EASTERN THAI CONSULTING 1992 CO., LTD.
SAHA GROUP INDUSTRIAL PARK, 683 MOO 11,
NONGKHAM, SIRACHA, CHONBURI 20230 THAILAND.

Location :
Ambient Temperature : (23.0 ± 3) °C
Pressure : (101.3 ± 3) kPa
Relative Humidity : (50.0 ± 20) %

Received Date : 29 APRIL 2024
Calibration Date : 16 MAY 2024
Date of Issue : 20 MAY 2024

Calibrated by : Nathakorn Pistupaisan

Approved by :
T. Petchurai
(Thanakul Petchurai)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

COPY

Calibration Method :

This equipment was calibrated by follow on IEC-60942-2003 Standard.
The sound pressure level, frequency and total distortion of the sound calibrator was measured using the reference microphone.

Condition of this result of calibration :

1. Reference Standard Instruments :

Instrument	Model	Serial No.	Cert. No.	Due Date
Waveform Generator	3351113	MY52302742	EF-0007-24	05-FEB-25
Digital Multimeter	33461A	MY53220104	EEL-BP 21/0267	13-FEB-25
Digital Multimeter	33461A	MY53220076	EEL-BP 20/0267	15-FEB-25
Digital Multimeter	33461A	MY60024273	EEL-BP 22/0267	15-FEB-25
Programmable Attenuator	MAT-1070	62100114	EF-0008-24	05-FEB-25
Condenser Microphone	4180	2977900	AA-1001-24	12-FEB-25
Measuring Amplifier	NA-42KAI	34560495	AA-3001-24	05-FEB-25
Audio Analyzer	AVR-3360A	V744B6069	EF-0009-24	09-FEB-25

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.
3. This certificate is traceable to the international system of unit maintained at :

- 3.1 National Institute of Metrology (Thailand).
- 3.2 Thailand Institute of Scientific and Technological Research (TISTR).

COPY
T. Petchurai



Result of calibration :

1. Sound pressure level

Specified sound pressure level (dB)	Measured value (dB)	Deviated value (dB)	Uncertainty (dB)	Acceptance limit (dB)
94	94.01	0.01	0.28	0.40

2. Frequency

Specified Frequency (Hz)	Measured value (Hz)	Deviated value (%)	Uncertainty (%)	Acceptance limit (%)
1000	1000.0	0.0	0.1	1.0

3. Total distortion


Measured value (%)	Uncertainty (%)	Acceptance limit (%)
0.31	0.10	3.0

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor $k = 2$ or any value following calculation providing a level of confidence of approximately 95 %

End of Calibration Certificate

COPY

S. Petchara



Cert. No. : ACL24141
Pages : 1 of 8

Calibration Certificate

Equipment : SOUND LEVEL METER
Manufacturer : RION
Model : NL-42A / Microphone UC-52 / Preamplifier NH-24
Serial No.: 00322754 / 196477 / 15486
ID No.:

Condition As Found : GOOD

Customer : EASTERN THAI CONSULTING 1992 CO., LTD.
SAHA GROUP INDUSTRIAL PARK, 683 MOO 11,
NONGKHAM, SIRACHA, CHONBURI 20230 THAILAND.

Location :
Ambient Temperature : (23.0 ± 3) °C
Pressure : (101.3 ± 3) kPa
Relative Humidity : (50.0 ± 20) %

Received Date : 29 APRIL 2024
Calibration Date : 13-17 MAY 2024
Date of Issue : 20 MAY 2024

Calibrated by : Nathakorn Pisutpaisan

Approved by :
(Thanakul Petchurai)

COPY

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

Calibration Procedure : CP-AC-01

Calibration Method :

This equipment was calibrated by follow on IEC-61672-3 (2013) Standard for sound level meter (SLM).
The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.

For tests results of each items were made by observation of each Instruments display and also with SLM's display.

Condition of this result of calibration :

1. Reference Standard Instruments :

Instrument	Model	Serial No.	Cert. No.	Due Date
Waveform Generator	33210A	MY48017076	EF-0009-4	05-FEB-25
Waveform Generator	33511B	MY52302742	EF-0007-24	05-FEB-25
Digital Multimeter	33461A	MY53220104	EEL.BP 21/0267	13-FEB-25
Digital Multimeter	33461A	MY53220076	EEL.BP 20/0267	15-FEB-25
Digital Multimeter	34461A	MY60024273	EEL.BP 22/0267	15-FEB-25
Programmable Attenuator	MAT-1070	62100114	EF-0008-24	05-FEB-25
Condenser Microphone	4180	2977900	AA-1001-24	12-FEB-25
Measuring Amplifier	NA-42KA1	34560495	AA-3001-24	05-FEB-25

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.
3. This certificate is traceable to the international system of unit maintained at :

- 3.1 National Institute of Metrology (Thailand).
- 3.2 Thailand Institute of Scientific and Technological Research (TISTR).

COPY

7. Petchurai

Summary of Measurement Result :

Parameter	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	0.2	N/A
2. Self-generated noise	0.2	N/A
3. Acoustical signal tests of frequency weightings		
125 Hz	0.3	0.6
1000 Hz	0.3	0.6
8000 Hz	0.3	0.7
4. Electrical signal tests of frequency weightings		
For 10 Hz to 4 kHz	0.3	0.6
For > 4 kHz to 10 kHz	0.3	0.7
For > 10 kHz to 20 kHz	-	1.0
5. Frequency and time weightings at 1 kHz	0.2	0.2
6. Long-term stability	0.1	0.1
7. Level linearity on the reference level range	0.2	0.3
8. Level linearity including the level range control	0.2	0.3
9. Tone burst response	0.2	0.3
10. Peak C sound level	0.2	0.35
11. Overload indication	0.2	0.25
12. High level stability	0.1	0.1

COPY

T. Petcha.

Result of calibration :

1. Absolute sensitivity

Reference Acoustic Signal (dB)	Measured Value (dB)	Deviation (dB)	Acceptance Limit (dB)
93.9 (93.98)	93.9	0.0	±0.3

2. Self-generated noise

2.1 Normal test

Measured Value (dB)
14.4

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Measured value (dB)
A - weight	10.8
C - weight	16.7
Flat	22.6

3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)		
	Flat	C-weight	A-weight
125	0.1	0.1	0.1
1000	0.0	0.0	0.0
8000	0.5	0.5	0.5

COPY

T. Petcha.

4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)		
	Flat	C-weight	A-weight
63	0.0	0.0	0.0
125	0.0	0.1	0.0
250	0.0	0.0	0.0
500	0.0	0.1	0.0
1000	0.0	0.0	0.0
2000	0.0	0.1	0.0
4000	0.0	0.1	0.0
8000	0.0	0.1	0.1

5. Frequency and time weightings at 1 kHz

5.1 Frequency weightings at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.2
C - weight	94.0	94.0	0.0	± 0.2
Flat	94.0	94.0	0.0	± 0.2

5.2 Time weighting at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	94.0	94.0	0.0	± 0.1
Slow	94.0	94.0	0.0	± 0.1
Leq	94.0	94.0	0.0	± 0.1

6. Long - term stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.1	0.1	± 0.3

7. Level linearity on the reference level range

Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
137.0	137.0	0.0	± 1.1
136.0	136.0	0.0	± 1.1
135.0	135.0	0.0	± 1.1
134.0	134.0	0.0	± 1.1
133.0	133.0	0.0	± 1.1
132.0	132.0	0.0	± 1.1
131.0	131.0	0.0	± 1.1
129.0	129.0	0.0	± 1.1
124.0	124.0	0.0	± 1.1
119.0	119.0	0.0	± 1.1
114.0	114.0	0.0	± 1.1
109.0	109.0	0.0	± 1.1
104.0	104.1	0.1	± 1.1
99.0	99.0	0.0	± 1.1
94.0	94.0	0.0	± 1.1
89.0	89.0	0.0	± 1.1
84.0	84.0	0.0	± 1.1
79.0	79.0	0.0	± 1.1
74.0	74.0	0.0	± 1.1
69.0	69.0	0.0	± 1.1
64.0	64.0	0.0	± 1.1
59.0	59.0	0.0	± 1.1
54.0	54.0	0.0	± 1.1
49.0	49.0	0.0	± 1.1
44.0	44.0	0.0	± 1.1
39.0	39.0	0.0	± 1.1
34.0	34.0	0.0	± 1.1
30.0	30.0	0.0	± 1.1
29.0	29.1	0.1	± 1.1
28.0	28.2	0.2	± 1.1
27.0	27.2	0.2	± 1.1
26.0	26.2	0.2	± 1.1
25.0	25.2	0.2	± 1.1

8. Level linearity including the level range control

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Auto	94.0	94.0	0.0	±1.1

9. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Cycle	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	0.25	1	108.0	108.0	0.0	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.1	0.1	±1.0
Slow	2	8	108.0	108.0	0.0	1.5 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
SEL	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.1	0.1	±1.0

10. Peak C sound level

Number of cycle in test signal	Anticipated Value (dB)	Measured Value, L _{peak} (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	±3.0
One	136.4	136.0	-0.4	±3.0

Number of cycle in test signal	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.1	0.1	±2.0
Positive half cycle	135.4	135.2	-0.2	±2.0
Negative half cycle	135.4	135.2	-0.2	±2.0

11. Overload indication

Measured value (dB)		Deviated Value (dB)	Acceptance Limits (dB)
Positive one-half cycle	Negative one-half cycle	0.0	±1.5
89.6	89.6		

12. High level stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor $k = 2$ or any value following calculation, providing a level of confidence of approximately 95 %

End of Calibration Certificate

COPY

7. Petch

COPY

7. Petch

Calibration Certificate

Equipment : SOUND LEVEL METER
Manufacturer : RION
Model : NL-42A / Microphone UC-52 / Preamplifier NH-24
Serial No.: 00322752 / 196475 / 15484
ID No.: -

Condition As Found : GOOD

Customer : EASTERN THAI CONSULTING 1992 CO., LTD.
SAHA GROUP INDUSTRIAL PARK, 683 MOO 11,
NONGKHAM, SIRACHA, CHONBURI 20230 THAILAND.

Location : -
Ambient Temperature : (23.0 ± 3) °C
Pressure : (101.3 ± 3) kPa
Relative Humidity : (50.0 ± 20) %

Received Date : 29 APRIL 2024
Calibration Date : 13-17 MAY 2024
Date of Issue : 20 MAY 2024

Calibrated by : Nathakorn Pisutpaisan

Approved by :

T. Petchurai

(Thanakul Petchurai)

COPY

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

Calibration Procedure : CP-AC-01

Calibration Method :

This equipment was calibrated by follow on IEC-61672-3 (2013) Standard for sound level meter (SLM).

The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anchoic chamber and Reference Standard Instruments.

For tests results of each items were made by observation of each Instruments display and also with SLM's display.

Condition of this result of calibration :

1. Reference Standard Instruments :

Instrument	Model	Serial No.	Cert. No.	Due Date
Waveform Generator	33210A	MY48017076	EF-0009-4	05-FEB-25
Waveform Generator	33511B	MY52302742	EF-0007-24	05-FEB-25
Digital Multimeter	33461A	MY53220104	EEL-BP 21/0267	13-FEB-25
Digital Multimeter	33461A	MY53220076	EEL-BP 20/0267	15-FEB-25
Digital Multimeter	34461A	MY60024273	EEL-BP 22/0267	15-FEB-25
Programmable Attenuator	MAT-1070	62100114	EF-0008-24	05-FEB-25
Condenser Microphone	4180	2977900	AA-1001-24	12-FEB-25
Measuring Amplifier	NA-42KAI	34560495	AA-3001-24	05-FEB-25

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is traceable to the international system of unit maintained at :

- 3.1 National Institute of Metrology (Thailand).
- 3.2 Thailand Institute of Scientific and Technological Research (TISTR).

COPY

T. Petchurai

Summary of Measurement Result :

Parameter	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	0.2	N/A
2. Self-generated noise	0.2	N/A
3. Acoustical signal tests of frequency weightings		
125 Hz	0.3	0.6
1000 Hz	0.3	0.6
8000 Hz	0.3	0.7
4. Electrical signal tests of frequency weightings		
For 10 Hz to 4 kHz	0.3	0.6
For > 4 kHz to 10 kHz	0.3	0.7
For > 10 kHz to 20 kHz	-	1.0
5. Frequency and time weightings at 1 kHz	0.2	0.2
6. Long - term stability	0.1	0.1
7. Level linearity on the reference level range	0.2	0.3
8. Level linearity including the level range control	0.2	0.3
9. Tone burst response	0.2	0.3
10. Peak C sound level	0.2	0.35
11. Overload indication	0.2	0.25
12. High level stability	0.1	0.1

COPY

T. Petch.

Result of calibration :

1. Absolute sensitivity

Reference Acoustic Signal (dB)	Measured Value (dB)	Deviation (dB)	Acceptance Limit (dB)
93.9 (93.98)	93.9	0.0	±0.3

2. Self-generated noise

2.1 Normal test

Measured Value (dB)
14.4

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Measured value (dB)
A - weight	10.8
C - weight	17.0
Flat	22.7

3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)		
	Flat	C-weight	A-weight
125	0.1	0.1	0.2
1000	0.0	0.0	0.0
8000	0.8	0.9	0.9

COPY

T. Petch.

4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)		
	Flat	C-weight	A-weight
63	0.0	-0.1	-0.1
125	0.0	0.0	0.0
250	0.0	0.0	0.0
500	0.0	0.1	0.0
1000	0.0	0.0	0.0
2000	0.0	0.1	0.1
4000	0.0	0.1	0.0
8000	0.1	0.1	0.1

5. Frequency and time weightings at 1 kHz

5.1 Frequency weightings at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.2
C - weight	94.0	94.0	0.0	± 0.2
Flat	94.0	94.0	0.0	± 0.2

5.2 Time weighting at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	94.0	94.0	0.0	± 0.1
Slow	94.0	94.0	0.0	± 0.1
Leq	94.0	94.0	0.0	± 0.1

6. Long - term stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.1	0.1	± 0.3

7. Level linearity on the reference level range

Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
137.0	137.0	0.0	± 1.1
136.0	136.0	0.0	± 1.1
135.0	135.1	0.1	± 1.1
134.0	134.1	0.1	± 1.1
133.0	133.0	0.0	± 1.1
132.0	132.0	0.0	± 1.1
131.0	131.0	0.0	± 1.1
129.0	129.0	0.0	± 1.1
124.0	124.0	0.0	± 1.1
119.0	119.1	0.1	± 1.1
114.0	114.0	0.0	± 1.1
109.0	109.0	0.0	± 1.1
104.0	104.1	0.1	± 1.1
99.0	99.0	0.0	± 1.1
94.0	94.0	0.0	± 1.1
89.0	89.0	0.0	± 1.1
84.0	84.0	0.0	± 1.1
79.0	79.0	0.0	± 1.1
74.0	74.0	0.0	± 1.1
69.0	69.0	0.0	± 1.1
64.0	64.0	0.0	± 1.1
59.0	59.0	0.0	± 1.1
54.0	54.0	0.0	± 1.1
49.0	49.0	0.0	± 1.1
44.0	44.0	0.0	± 1.1
39.0	38.9	-0.1	± 1.1
34.0	33.9	-0.1	± 1.1
30.0	29.9	-0.1	± 1.1
29.0	28.9	-0.1	± 1.1
28.0	27.9	-0.1	± 1.1
27.0	26.9	-0.1	± 1.1
26.0	25.9	-0.1	± 1.1
25.0	24.8	-0.2	± 1.1

COPY

T. Retehn

COPY

T. Retehn

Cert. No. : ACL24139

Job No. : VC67AC0083

Pages : 7 of 8

Cert. No. : ACL24139

Job No. : VC67AC0083

Pages : 8 of 8

8. Level linearity including the level range control

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Auto	94.0	94.0	0.0	±1.1

9. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Cycle	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	116.9	-0.1	1.0 ; -2.5
	200	800	134.0	134.0	0.0	±1.0
Slow	2	8	108.0	107.9	-0.1	1.5 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
SEL	0.25	1	99.0	98.8	-0.2	1.5 ; -5.0
	2	8	108.0	107.9	-0.1	1.0 ; -2.5
	200	800	128.0	128.0	0.0	±1.0

10. Peak C sound level

Number of cycle in test signal	Anticipated Value (dB)	Measured Value, Lepeak (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	±3.0
One	136.4	135.6	-0.8	±3.0

Number of cycle in test signal	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	±2.0
Positive half cycle	135.4	135.1	-0.3	±2.0
Negative half cycle	135.4	135.1	-0.3	±2.0

11. Overload indication

Measured value (dB)		Deviated Value (dB)	Acceptance Limits (dB)
Positive one-half cycle	Negative one-half cycle	0.0	±1.5
89.5	89.5		

12. High level stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor $k = 2$ or any value following calculation, providing a level of confidence of approximately 95 %


End of Calibration Certificate

COPY

COPY

T. P. P.

T. P. P.



Calibration Certificate

Equipment : SOUND LEVEL METER
Manufacturer : RION
Model : NL-42A / Microphone UC-52 / Preamplifier NH-24
Serial No.: 00322747 / 196470 / 15479
ID No.:

Condition As Found : GOOD

Customer : EASTERN THAI CONSULTING 1992 CO., LTD.
SAHA GROUP INDUSTRIAL PARK, 683 MOO 11,
NONGKHAM, SIRACHA, CHONBURI 20230 THAILAND.

Location :
Ambient Temperature : (23.0 ± 3) °C
Pressure : (101.3 ± 3) kPa
Relative Humidity : (50.0 ± 20) %

Received Date : 29 APRIL 2024
Calibration Date : 13-17 MAY 2024
Date of Issue : 20 MAY 2024

Calibrated by : Nathakorn Pisutpaisan

Approved by :
(Thanakul Petchurai)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

COPY



Calibration Procedure : CP-AC-01

Calibration Method :

This equipment was calibrated by follow on IEC-61672-3 (2013) Standard for sound level meter (SLM).
The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.

For tests results of each items were made by observation of each Instruments display and also with SLM's display.

Condition of this result of calibration :

1. Reference Standard Instruments :

Instrument	Model	Serial No.	Cert. No.	Due Date
Waveform Generator	33210A	MY48017076	EF-0009-4	05-FEB-25
Waveform Generator	33511B	MY52302742	EF-0007-24	05-FEB-25
Digital Multimeter	33461A	MY53220104	EEL_BP 21/0267	13-FEB-25
Digital Multimeter	33461A	MY53220076	EEL_BP 20/0267	15-FEB-25
Digital Multimeter	34461A	MY60024273	EEL_BP 22/0267	15-FEB-25
Programmable Attenuator	MAT-1070	62100114	EF-0008-24	05-FEB-25
Condenser Microphone	4180	2977900	AA-1001-24	12-FEB-25
Measuring Amplifier	NA-42KAI	34560495	AA-3001-24	05-FEB-25

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.
3. This certificate is traceable to the international system of unit maintained at :

- 3.1 National Institute of Metrology (Thailand).
- 3.2 Thailand Institute of Scientific and Technological Research (TISTR).

COPY

Summary of Measurement Result :

Parameter	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	0.2	N/A
2. Self-generated noise	0.2	N/A
3. Acoustical signal tests of frequency weightings		
125 Hz	0.3	0.6
1000 Hz	0.3	0.6
8000 Hz	0.3	0.7
4. Electrical signal tests of frequency weightings		
For 10 Hz to 4 kHz	0.3	0.6
For > 4 kHz to 10 kHz	0.3	0.7
For > 10 kHz to 20 kHz	-	1.0
5. Frequency and time weightings at 1 kHz	0.2	0.2
6. Long - term stability	0.1	0.1
7. Level linearity on the reference level range	0.2	0.3
8. Level linearity including the level range control	0.2	0.3
9. Tone burst response	0.2	0.3
10. Peak C sound level	0.2	0.35
11. Overload indication	0.2	0.25
12. High level stability	0.1	0.1

COPY

g. petch.

Result of calibration :

1. Absolute sensitivity

Reference Acoustic Signal (dB)	Measured Value (dB)	Deviation (dB)	Acceptance Limit (dB)
93.9 (93.98)	93.9	0.0	±0.3

2. Self-generated noise

2.1 Normal test

Measured Value (dB)
14.8

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Measured value (dB)
A - weight	11.3
C - weight	17.6
Flat	23.3

3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)		
	Flat	C-weight	A-weight
125	0.1	0.1	0.1
1000	0.0	0.0	0.0
8000	0.3	0.4	0.4
			Acceptance Limits
			± 1.5
			± 1.0
			±5.0

COPY

g. petch.

4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)		
	Flat	C-weight	A-weight Acceptance Limits
63	0.0	0.0	±2.0
125	0.0	0.1	±1.5
250	0.0	0.0	±1.5
500	0.0	0.1	±1.5
1000	0.0	0.0	±1.0
2000	0.0	0.1	±2.0
4000	0.0	0.1	±3.0
8000	0.0	0.1	±5.0

5. Frequency and time weightings at 1 kHz

5.1 Frequency weightings at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.2
C - weight	94.0	94.0	0.0	± 0.2
Flat	94.0	94.0	0.0	± 0.2

5.2 Time weighting at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	94.0	94.0	0.0	± 0.1
Slow	94.0	94.0	0.0	± 0.1
Leq	94.0	94.0	0.0	± 0.1

6. Long - term stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.1	0.1	± 0.3

7. Level linearity on the reference level range

Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
137.0	137.0	0.0	± 1.1
136.0	136.0	0.0	± 1.1
135.0	135.0	0.0	± 1.1
134.0	134.0	0.0	± 1.1
133.0	133.0	0.0	± 1.1
132.0	132.0	0.0	± 1.1
131.0	131.0	0.0	± 1.1
129.0	129.0	0.0	± 1.1
124.0	124.0	0.0	± 1.1
119.0	119.0	0.0	± 1.1
114.0	114.0	0.0	± 1.1
109.0	109.0	0.0	± 1.1
104.0	104.1	0.1	± 1.1
99.0	99.0	0.0	± 1.1
94.0	94.0	0.0	± 1.1
89.0	89.0	0.0	± 1.1
84.0	84.0	0.0	± 1.1
79.0	79.0	0.0	± 1.1
74.0	74.0	0.0	± 1.1
69.0	69.0	0.0	± 1.1
64.0	64.0	0.0	± 1.1
59.0	59.0	0.0	± 1.1
54.0	54.0	0.0	± 1.1
49.0	49.0	0.0	± 1.1
44.0	44.0	0.0	± 1.1
39.0	39.0	0.0	± 1.1
34.0	34.0	0.0	± 1.1
30.0	30.0	0.0	± 1.1
29.0	29.0	0.0	± 1.1
28.0	28.0	0.0	± 1.1
27.0	27.0	0.0	± 1.1
26.0	26.0	0.0	± 1.1
25.0	25.0	0.0	± 1.1

COPY
7. Petha

8. Level linearity including the level range control

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Auto	94.0	94.0	0.0	±1.1

9. Tone burst response

Time Weighting	Tone burst duration, T _b (ms)	Cycle	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	0.25	1	108.0	108.0	0.0	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.1	0.1	±1.0
Slow	2	8	108.0	108.0	0.0	1.5 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
SEL	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.1	0.1	±1.0

10. Peak C sound level

Number of cycle in test signal	Anticipated Value (dB)	Measured Value, L _{peak} (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	±3.0
One	136.4	135.3	-1.1	±3.0

Number of cycle in test signal	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.1	0.1	±2.0
Positive half cycle	135.4	135.2	-0.2	±2.0
Negative half cycle	135.4	135.2	-0.2	±2.0

11. Overload indication

Measured value (dB)		Deviated Value (dB)	Acceptance Limits (dB)
Positive one-half cycle	Negative one-half cycle		
89.6	89.5	-0.1	±1.5

12. High level stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	137.1	137.0	0.1	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor $k = 2$ or any value following calculation providing a level of confidence of approximately 95 %


End of Calibration Certificate

COPY

COPY

T. Petch

T. Petch



Cert. No. : ACC24014
Pages : 1 of 3

Calibration Certificate

Equipment : SOUND CALIBRATOR

Manufacturer : RION

Model : NC-75

Serial No.: 34302326

ID No.: -

Condition As Found : GOOD

Customer : EASTERN THAI CONSULTING 1992 CO., LTD.
SAHA GROUP INDUSTRIAL PARK, 683 MOO 11,
NONGKHAM, SIRACHA, CHONBURI 20230 THAILAND.


Location :
Ambient Temperature : (23.0 ± 3) °C
Pressure : (101.3 ± 3) kPa
Relative Humidity : (50.0 ± 20) %

Received Date : 29 APRIL 2024
Calibration Date : 16 MAY 2024
Date of Issue : 20 MAY 2024

Calibrated by : Nathakorn Pisutpaisan

Approved by :
(Thanakul Petchurai)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory

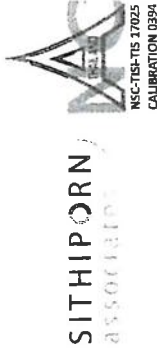

Cert. No. : ACC24014
Job No. : VC67AC0083
Pages : 2 of 3

Calibration Procedure : CP-AC-03

Calibration Method :

This equipment was calibrated by follow on IEC-60942-2003 Standard.

The sound pressure level, frequency and total distortion of the sound calibrator was measured using the reference microphone.

Condition of this result of calibration :

1. Reference Standard Instruments :

Instrument	Model	Serial No.	Cert. No.	Due Date
Waveform Generator	33511B	MY52302742	EF-0007-24	05-FEB-25
Digital Multimeter	33461A	MY53220104	EEL-BP 21/0267	13-FEB-25
Digital Multimeter	33461A	MY53220076	EEL-BP 20/0267	15-FEB-25
Digital Multimeter	33461A	MY60024273	EEL-BP 22/0267	15-FEB-25
Programmable Attenuator	MAT-1070	62100114	EF-0008-24	05-FEB-25
Condenser Microphone	4180	2977900	AA-1001-24	12-FEB-25
Measuring Amplifier	NA-42KAI	34560495	AA-3001-24	05-FEB-25
Audio Analyzer	AVR-3360A	V744B6069	EF-0009-24	09-FEB-25

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.
3. This certificate is traceable to the international system of unit maintained at :

- 3.1 National Institute of Metrology (Thailand).
- 3.2 Thailand Institute of Scientific and Technological Research (TISTR).

COPY

Cert. No. : ACC24014
Job No. : VC67ACW083
Pages : 3 of 3

Result of calibration :

1. Sound pressure level

Specified sound pressure level (dB)	Measured value (dB)	Deviated value (dB)	Uncertainty (dB)	Acceptance limit (dB)
94	94.01	0.01	0.28	0.40

2. Frequency

Specified Frequency (Hz)	Measured value (Hz)	Deviated value (%)	Uncertainty (%)	Acceptance limit (%)
1000	1000.0	0.0	0.1	1.0

3. Total distortion

Measured value (%)	Uncertainty (%)	Acceptance limit (%)
0.31	0.10	3.0

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor $k = 2$
or any value following calculation, providing a level of confidence of approximately 95 %

End of Calibration Certificate

COPY

S. Petch



THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-67/0251

MTC No. EEL. BP. 8/0267

CALIBRATION CERTIFICATE

Submitted by : Eastern Thai Consulting 1992 Co., Ltd.

Address : 683 Moo 11 Sukaphibal 8 Rd., Nongkham, Sriracha, Chonburi 20230

Calibrated at : Electrical and Electronic Standards Laboratory, Industrial Metrology and Testing Service Centre.

Soi 1C, Bangpoo Industrial Estate, Sukhumvit Rd., A.Muang, Samutprakan 10280.

Instrument Calibrated :

Description		Ambient Environment		
Manufacturer	Cirrus	Sound Level Meter	Temperature : (23 ± 3) °C	
			Relative Humidity : (50 ± 15) %	
		Model	Ambient Pressure : (101.325±1.5) kPa	
Serial No.		: G301638		
Microphone		: MK216 No.412753E		
Preamplifier		: 10402F		

Standards used :

1. Band Pass Filter Wavetek 752A S/N 90010494.
2. Condenser Microphone Brüel&Kjær 4180 S/N 2889871.
3. Decade Attenuator Ando AL-205 S/N 00464602.
4. Function/Arbitrary Waveform Generator Agilent 33220A S/N MY44042668.
5. Digital Function Synthesizer NF Electronic Instruments DF-193A S/N 122037.
6. Digital Multimeter Fluke 8520A S/N 4985007.
7. Multifunction Acoustic Calibrator Brüel&Kjær 4226 S/N 2810358 with Coupler UAD915 S/N 2810358
8. Measuring Amplifier Brüel&Kjær 2636 S/N 1537484.

Date of Receipt : 5 Feb. 2024

Date of Calibration : 1 Mar. 2024

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

The results relate only to the items tested/calibrated or value assigned.

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9000
Fax. (66) 0 2577 9009
E-mail : rumalai@tistr.or.th Website:www.tistr.or.th

Office/Laboratory
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,
Amphoe Muang, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
Fax. (66) 0 2323 9165
E-mail : mtc@tistr.or.th

FM.BL.MTC.002 Rev.1



THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-67/0251

MTC No. EEL. BP. 8/0267

9. Power Amplifier Brüel&Kjær 2706 S/N 1517650.
10. Speaker Tannoy Limited, Great Britain British Patent No. 215300.
11. Digital Multimeter Agilent 34401A S/N MY44005560.
12. Programmable Attenuator Tamagawa TPA-303A S/N 2212.

Calibration Procedure :

This instrument was calibrated by using calibration procedures no CP-102-02 and CP-102-03, which were based on IEC 61672-3 Electroacoustics - Sound Level Meters - Part 3 : Periodic tests (2013). These calibration procedures were related to the electrical and acoustic signal tests. The electrical signal test was carried out with the direct measurement method. The acoustic signal test was performed in an anechoic room with the comparison measurement method.

This instrument has been calibrated against standards maintained at the Electrical and Electronic Standards Laboratory (EEL), which are traceable to the International System of Units through the National Institute of Metrology (Thailand).

The information on actual reading is attached herewith and the uncertainty limits quoted refer to the measured values only.

The reported expanded uncertainty is based upon a standard uncertainty multiplied by a coverage factor k=2, providing a level of confidence of approximately 95%.

Date of Calibration : 1 Mar. 2024

2 / 5

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9000
Fax. (66) 0 2577 9009
E-mail : rumalai@tistr.or.th Website:www.tistr.or.th

Office/Laboratory
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,
Amphoe Muang, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
Fax. (66) 0 2323 9165
E-mail : mtc@tistr.or.th

FM.BL.MTC.002 Rev.

1. Absolute Sensitivity

Reference Acoustic Signal (dB)	Measured value (dB)		Deviation value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
	Before adjust	After adjust				
93.70	93.6	93.7	0.0	1.0	0.48	N/A

Note: The external calibration adjustment was firstly performed. The internal calibration adjustment was then completed at the display of 93.7 dB.

2. Self-generated noise

2.1 Normal test

Measured value (dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
19.8	0.10	N/A

2.2 The microphone of the sound level meter was replaced by electrical signal input device

Frequency Weighting	Measured value (dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
A-Weight	under-range	-	N/A
C-Weight	17.2	0.10	N/A
Flat	28.6	0.10	N/A

Note: The under-range means that the indicator cannot display for setting the range of 20-140 dB.

Date of Calibration : 1 Mar. 2024

3
COPY

The results relate only to the items tested/calibrated or value assigned. Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang, Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9000
Fax. (66) 0 2577 9009
E-mail : rumpa@tistr.or.th Website: www.tistr.or.th

Office/Laboratory
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road, Amphoe Muang, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
Fax. (66) 0 2323 9165
E-mail : mtc@tistr.or.th

Office
196 Phahonyothin Road, Chatuchak, Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-3C ext. 5219, 5225, 5217
Fax. (66) 0 2579 8592
E-mail : sumalee@tistr.or.th

FM.BLMTC.002 Rev.1

Request No. 21-67/0251

MTC No. EEL. BP. 8/0267

3. Acoustical signal test of frequency weightings

Frequency (Hz)	Deviation from frequency response curve (dB)			Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
	A-weight	C-weight	Flat			
125	0.7	0.5	0.5	1.5	0.45	0.6
1 000	-0.4	-0.3	-0.3	1.0	0.45	0.6
8 000	-2.8	-2.7	-2.4	5.0	0.45	0.7

4. Electrical signal test of frequency weightings

Frequency (Hz)	Deviation from frequency response curve (dB)			Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
	A-weight	C-weight	Flat			
63	0.5	0.0	0.1	2.0	0.20	0.6
125	0.3	0.0	0.0	1.5	0.20	0.6
250	0.2	0.0	-0.1	1.5	0.20	0.6
500	0.1	0.0	-0.1	1.5	0.20	0.6
1 000	0.0	0.0	0.0	1.0	0.20	0.6
2 000	-0.1	0.0	0.0	2.0	0.20	0.6
4 000	-0.3	-0.2	0.0	3.0	0.20	0.6
8 000	-0.5	-0.3	-0.1	5.0	0.20	0.7

Date of Calibration : 1 Mar. 2024

4 / 9

3
COPY

The results relate only to the items tested/calibrated or value assigned. Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang, Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9000
Fax. (66) 0 2577 9009
E-mail : rumpa@tistr.or.th Website: www.tistr.or.th

Office/Laboratory
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road, Amphoe Muang, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
Fax. (66) 0 2323 9165
E-mail : mtc@tistr.or.th

Office
196 Phahonyothin Road, Chatuchak, Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
Fax. (66) 0 2579 8592
E-mail : sumalee@tistr.or.th

FM.BLMTC.002 Rev.1

Request No. 21-67/0251

MTC No. EEL. BP. 8/0267

5. Long-term stability

Time	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (\pm dB)	Uncertainty (\pm dB)	Maximum-permitted uncertainty of measurement (\pm dB)
Begin	94.0	0.0	0.3	0.10	0.1
End	94.0				

6. Frequency and time weightings at 1 kHz

6.1 Frequency weightings at 1 kHz

Frequency Weighting	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (\pm dB)	Uncertainty (\pm dB)	Maximum-permitted uncertainty of measurement (\pm dB)
A-weight	94.0	0.0	0.2	0.20	0.2
C-weight	94.0	0.0	0.2	0.20	0.2
Flat	94.0	0.0	0.2	0.20	0.2

6.2 Time weightings at 1 kHz

Frequency Weighting	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (\pm dB)	Uncertainty (\pm dB)	Maximum-permitted uncertainty of measurement (\pm dB)
Fast	94.0	0.0	0.1	0.20	0.2
Slow	94.0	0.0	0.1	0.20	0.2
Leq	94.0	0.0	0.1	0.20	0.2

Date of Calibration : 1 Mar. 2024

The results relate only to the items tested/calibrated or value assigned. Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

Head Office 35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang, Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9000
Fax. (66) 0 2577 9009
E-mail : rumpa@tistr.or.th Website: www.tistr.or.th

Office/Laboratory Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road, Amphoe Muang, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
Fax. (66) 0 2323 9165
E-mail : mtc@tistr.or.th

Office 196 Phahonyothin Road, Chatuchak Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
Fax. (66) 0 2579 8592
E-mail : sumalee@tistr.or.th

FM.BLMTC.002 Rev.1

Request No. 21-67/0251

MTC No. EEL. BP. 8/0267

7. Level linearity on the reference level range

Anticipated value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (\pm dB)	Uncertainty (\pm dB)	Maximum-permitted uncertainty of measurement (\pm dB)
138	138.0	0.0	1.1	0.30	0.3
134	134.0	0.0	1.1	0.30	0.3
129	129.0	0.0	1.1	0.30	0.3
124	124.0	0.0	1.1	0.30	0.3
119	119.0	0.0	1.1	0.30	0.3
114	114.0	0.0	1.1	0.30	0.3
109	109.0	0.0	1.1	0.30	0.3
104	104.0	0.0	1.1	0.30	0.3
99	99.0	0.0	1.1	0.30	0.3
94	94.0	0.0	1.1	0.30	0.3
89	89.0	0.0	1.1	0.30	0.3
84	83.9	-0.1	1.1	0.30	0.3
79	79.0	0.0	1.1	0.30	0.3
74	74.0	0.0	1.1	0.30	0.3
69	69.0	0.0	1.1	0.30	0.3
64	63.9	-0.1	1.1	0.30	0.3
59	58.9	-0.1	1.1	0.30	0.3
54	53.9	-0.1	1.1	0.30	0.3

Date of Calibration : 1 Mar. 2024

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

Head Office 35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang, Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9000
Fax. (66) 0 2577 9009
E-mail : rumpa@tistr.or.th Website: www.tistr.or.th

Office/Laboratory Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road, Amphoe Muang, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
Fax. (66) 0 2323 9165
E-mail : mtc@tistr.or.th

Office 196 Phahonyothin Road, Chatuchak Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
Fax. (66) 0 2579 8592
E-mail : sumalee@tistr.or.th

FM.BLMTC.002 Rev.1

7. Level linearity on the reference level range (cont.)

Anticipated value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
49	48.9	-0.1	1.1	0.30	0.3
44	43.9	-0.1	1.1	0.30	0.3
39	38.9	-0.1	1.1	0.30	0.3
34	33.9	-0.1	1.1	0.30	0.3
29	28.9	-0.1	1.1	0.30	0.3
28	28.0	0.0	1.1	0.30	0.3
27	27.0	0.0	1.1	0.30	0.3
26	25.9	-0.1	1.1	0.30	0.3
25	25.0	0.0	1.1	0.30	0.3

8. Level linearity including the level range control

At reference sound level on the reference level range

Range	Anticipated value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
20-140	94.0	94.0	0.0	1.1	0.30	0.3

Date of Calibration : 1 Mar. 2024

The results relate only to the items tested/calibrated or value assigned.
Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

8. Level linearity including the level range control

At reference level at 5 dB greater than the under-range on a level range

Range	Anticipated value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
20-140	25	25.0	0.0	1.1	0.30	0.3

9. Tone burst response

Time Weighting	Toneburst Duration, Tb(ms)	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Fast	200	136.0	0.0	±1.0	0.20	0.3
	2	118.8	-0.2	+1.0; -2.5	0.20	0.3
	0.25	109.8	-0.2	+1.5; -5.0	0.20	0.3
Slow	200	129.5	-0.1	±1.0	0.20	0.3
	2	109.9	-0.1	+1.0; -5.0	0.20	0.3
	0.25	130.0	0.0	±1.0	0.20	0.3
SEL	2	110.0	0.0	+1.0; -2.5	0.20	0.3
	0.25	100.9	-0.1	+1.5; -5.0	0.20	0.3

Date of Calibration : 1 Mar. 2024

The results relate only to the items tested/calibrated or value assigned.
Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

Request No. 21-67/0251

MTC No. EEL. BP. 8/0267

10. Peak C sound level

Number of cycles in test signal	Anticipated value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Complete cycle	135.4	135.6	0.2	3.0	0.20	0.35
Positive half cycle	134.4	134.3	-0.1	2.0	0.20	0.35
Negative half cycle	134.4	134.3	-0.1	2.0	0.20	0.35

11. Overload indication

Measured value (dB)		Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Positive one-half cycle	Negative one-half cycle	value (dB)	limit class 2 (±dB)	(±dB)	of measurement (±dB)
138.6	138.6	0.0	1.5	0.20	0.25

12. High-level stability

Time	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Begin	139.0	0.0	0.3	0.10	0.1
End	139.0				

Calibrated by : 
(Mr. Witawat Supanich)

Approved by : 
(Mr. Panyat Chumpha)
Director

Electrical and Electronics Standards Laboratory
Industrial Metrology and Testing Service Centre

Date of Calibration : 1 Mar. 2024
Date of Issue : 4 Mar. 2024

Ref : 2011267020500502003

End of Certificate

9 / 9

Cert. No. : ACL24148
Pages : 1 of 9

Calibration Certificate

Equipment : SOUND LEVEL METER
Manufacturer : CIRRUS
Model : CR-172 A / Microphone PMP21 / Preamplifier -
Serial No.: G301660 / 230007 / 10093F
ID No.: -

Condition As Found : GOOD

Customer : EASTERN THAI CONSULTING 1992 CO., LTD.
SAHA GROUP INDUSTRIAL PARK, 683 MOO 11,
NONGKHAM, SIRACHA, CHONBURI 20230 THAILAND.

Location : -
Ambient Temperature : (23.0 ± 3) °C
Pressure : (101.3 ± 3) kPa
Relative Humidity : (50.0 ± 20) %

Received Date : 29 APRIL 2024
Calibration Date : 27 -28 MAY 2024
Date of Issue : 29 MAY 2024

Calibrated by : Nathakorn Pisutpaisan

Approved by :
(Thanakul Petchurai)

COPY

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

Cert. No. : ACL24148
Job No. : VC67AC0083
Pages : 2 of 9

Calibration Procedure : CP-AC-02

Calibration Method :

This equipment was calibrated by follow on IEC-61672-3 (2013) Standard for sound level meter (SLM).
The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.

For tests results of each items were made by observation of each Instruments display and also with SLM's display.

Condition of this result of calibration :

1. Reference Standard Instruments :

Instrument	Model	Serial No.	Cert. No.	Due Date
Waveform Generator	33210A	MY48017076	EF-0009-4	05-FEB-25
Waveform Generator	33511B	MY52302742	EF-0007-24	05-FEB-25
Digital Multimeter	33461A	MY53220104	EEL-BP 21/0267	13-FEB-25
Digital Multimeter	33461A	MY53220076	EEL-BP 20/0267	15-FEB-25
Digital Multimeter	34461A	MY60024273	EEL-BP 22/0267	15-FEB-25
Programmable Attenuator	MAT-1070	62100114	EF-0008-24	05-FEB-25
Condenser Microphone	4180	2977900	AA-1001-24	12-FEB-25
Measuring Amplifier	NA-42KAI	34560495	AA-3001-24	05-FEB-25

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is traceable to the international system of unit maintained at :

- 3.1 National Institute of Metrology (Thailand).
- 3.2 Thailand Institute of Scientific and Technological Research (TISTR).

COPY

T. Petchurai

Summary of Measurement Result :

Parameter	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	0.2	N/A
2. Self-generated noise	0.2	N/A
3. Acoustical signal tests of frequency weightings		
125 Hz	0.3	0.6
1000 Hz	0.3	0.6
8000 Hz	0.3	0.7
4. Electrical signal tests of frequency weightings		
For 10 Hz to 4 kHz	0.3	0.6
For > 4 kHz to 10 kHz	0.3	0.7
For > 10 kHz to 20 kHz	-	1.0
5. Frequency and time weightings at 1 kHz	0.2	0.2
6. Long - term stability	0.1	0.1
7. Level linearity on the reference level range	0.2	0.3
8. Level linearity including the level range control	0.2	0.3
9. Tone burst response	0.2	0.3
10. Peak C sound level	0.2	0.35
11. Overload indication	0.2	0.25
12. High level stability	0.1	0.1

COPY

T. Petch.

Result of calibration :

1. Absolute sensitivity

Reference Acoustic Signal (dB)	Measured Value (dB)	Deviation (dB)	Acceptance Limit (dB)
93.9 (93.94)	94.0	0.0	±0.3

2. Self-generated noise

2.1 Normal test

Measured Value (dB)
16.0

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Measured value (dB)
A - weight	14.4
C - weight	14.7
Flat	26.6

3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)		
	Flat	C-weight	A-weight
125	-0.3	-0.2	0.1
1000	-0.2	-0.2	-0.2
8000	0.0	-0.3	-0.5
			Acceptance Limits
			± 1.5
			± 1.0
			± 5.0

COPY

T. Petch.

Cert. No. : ACL24148

Job No. : VC67AC0083

Pages : 5 of 9

Cert. No. : ACL24148

Job No. : VC67AC0083

Pages : 6 of 9

4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)		
	Flat	C-weight	A-weight
63	0.2	0.0	0.4
125	0.1	0.0	0.2
250	0.1	0.0	0.2
500	0.1	0.0	0.1
1000	0.0	0.0	0.0
2000	0.1	-0.1	-0.2
4000	0.0	-0.2	-0.4
8000	-0.1	-0.4	-0.6

5. Frequency and time weightings at 1 kHz

5.1 Frequency weightings at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.2
C - weight	94.0	94.0	0.0	± 0.2
Flat	94.0	93.9	-0.1	± 0.2

5.2 Time weighting at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	94.0	94.0	0.0	± 0.1
Slow	94.0	94.0	0.0	± 0.1
Leq	94.0	94.0	0.0	± 0.1

6. Long - term stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.3

7. Level linearity on the reference level range

Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
133.0	133.0	0.0	± 1.1
132.0	132.0	0.0	± 1.1
131.0	131.0	0.0	± 1.1
130.0	130.0	0.0	± 1.1
129.0	129.0	0.0	± 1.1
124.0	124.0	0.0	± 1.1
119.0	119.0	0.0	± 1.1
114.0	114.0	0.0	± 1.1
109.0	109.0	0.0	± 1.1
104.0	104.0	0.0	± 1.1
99.0	99.0	0.0	± 1.1
94.0	94.0	0.0	± 1.1
89.0	89.0	0.0	± 1.1
84.0	83.9	-0.1	± 1.1
79.0	79.0	0.0	± 1.1
74.0	74.0	0.0	± 1.1
69.0	69.0	0.0	± 1.1
64.0	64.0	0.0	± 1.1
59.0	59.0	0.0	± 1.1
54.0	54.0	0.0	± 1.1
49.0	49.0	0.0	± 1.1
44.0	44.0	0.0	± 1.1
39.0	39.0	0.0	± 1.1
34.0	34.0	0.0	± 1.1
29.0	29.0	0.0	± 1.1

COPY

COPY

7. Reten

7. Reten

8. Level linearity including the level range control

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
130	94.0	94.0	0.0	±1.1

Level linearity on each level range

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
130	29.0	29.0	0.0	±1.1

9. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Cycle	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	116.9	-0.1	1.0 ; -2.5
	200	800	134.0	134.0	0.0	±1.0
Slow	2	8	108.0	108.0	0.0	1.5 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
SEL	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.0	0.0	±1.0

10. Peak C sound level

Number of cycle in test signal	Anticipated Value (dB)	Measured Value, Lcpeak (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	130.0	130.0	0.0	±3.0
One	133.4	133.6	0.2	±3.0

Number of cycle in test signal	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	130.0	130.0	0.0	±2.0
Positive half cycle	132.4	132.3	-0.1	±2.0
Negative half cycle	132.4	132.3	-0.1	±2.0

11. Overload indication

Measured value (dB)		Deviated Value (dB)	Acceptance Limits (dB)
Positive one-half cycle	Negative one-half cycle	0.1	±1.5
84.6	84.7		

COPY

Z. Petch

COPY

Z. Petch

Cert. No. : ACL24148
Job No. : VC67AC0083
Pages : 9 of 9


12. High level stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor $k = 2$
or any value following calculation, providing a level of confidence of approximately 95 %

_____ End of Calibration Certificate _____





CERTIFICATE OF CALIBRATION

ISSUED BY

Cirrus Research plc

DATE OF ISSUE

19 January 2024

CERTIFICATE NUMBER

206870

CERTIFICATE OF CALIBRATION

Certificate Number:

206870

Page

2 of 2



Cirrus Research plc

Acoustic House

Bridlington Road

Hunmanby

North Yorkshire

YO14 0PH

United Kingdom

Page 1 of 2

Approved signatory

N.Smith

Electronically signed:



Dosemeter : IEC 61252-1993+A1:2000

Instrument information

Manufacturer:

Cirrus Research plc

Model:

CR:110A

Serial number:

CB1365

Firmware version:

5.4

Notes:

Eastern Thai Consulting 1992 Co.,Ltd.
683 Moo.11, Sukaphibai 8 Rd., Nongkham,
Sriracha, Chonburi 20230

Test summary

Date of calibration:

19 January 2024

The calibration was performed respecting the requirements of ISO/IEC 17025:2017.

The dosimeter submitted for testing successfully completed the periodic tests of IEC 61252-1993+A1:2000.

The dosimeter submitted for testing conforms to the specifications in IEC 61252-1993+A1:2000.

Test equipment

Equipment	Manufacturer	Model	Serial number
Signal Generator	KEYSIGHT	33511B	MY58001553
Attenuator	Cirrus Research	ZE:952	78713
Environmental Monitor	Comet	T7510	16966334
doseBadge Reader	Cirrus Research plc	RC:110A	100498

Notes

This certificate provides traceability of measurement to the SI system of units and/or to units of measurement realised at the National Physical Laboratory or other recognised national metrology institutes. This certificate may not be reproduced other than in full, except with the prior written approval of the issuing laboratory. The results within this certificate relate only to the items calibrated. The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor k=2, providing a coverage probability of approximately 95%.

Environmental conditions

The following conditions were recorded at the time of the test:

Before

Pressure: 99.92 kPa

Temperature: 21.7 °C

Humidity: 33.2 %

After

Pressure: 99.96 kPa

Temperature: 21.8 °C

Humidity: 34.2 %

Test results summary


Test	Result
Linearity	Complies
Short Duration	Complies
Overload Latching	Complies
Frequency weighting	Complies
Absolute Acoustic Sensitivity	Complies

COPY

COPY

CERTIFICATE OF CALIBRATION

ISSUED BY Cirrus Research plc
DATE OF ISSUE 19 January 2024 CERTIFICATE NUMBER 206878



Cirrus Research plc
Acoustic House
Bridlington Road
Hunmanby
North Yorkshire
YO14 0PH
United Kingdom

Page 1 of 2

Approved signatory
N Smith
Electronically signed:

Dosimeter : IEC 61252-1993+A1:2000

Instrument information

Manufacturer: Cirrus Research plc Notes: Eastern Thai Consulting 1992 Co., Ltd.
Model: CR:110A 683 Moo.11, Sukaphibal 8 Rd., Nongkham,
Serial number: CB0641 Sriracha, Chonburi 20230
Firmware version: 5.4

Test summary

Date of calibration: 19 January 2024
The calibration was performed respecting the requirements of ISO/IEC 17025:2017.
The dosimeter submitted for testing successfully completed the periodic tests of IEC 61252-1993+A1:2000.
The dosimeter submitted for testing conforms to the specifications in IEC 61252-1993+A1:2000.

Test equipment

Equipment	Manufacturer	Model	Serial number
Signal Generator	KEYSIGHT	33511B	MY58001553
Attenuator	Cirrus Research	ZE:952	78713
Environmental Monitor	Comet	T7510	16966334
doseBadge Reader	Cirrus Research plc	RC:110A	100498

Notes

This certificate provides traceability of measurement to the SI system of units and/or to units of measurement realised at the National Physical Laboratory or other recognised national metrology institutes. This certificate may not be reproduced other than in full, except with the prior written approval of the issuing laboratory. The results within this certificate relate only to the items calibrated. The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor k=2, providing a coverage probability of approximately 95%.

CERTIFICATE OF CALIBRATION

Certificate Number:
206878
Page 2 of 2

Environmental conditions

The following conditions were recorded at the time of the test:

Before Pressure: 100.96 kPa Temperature: 21.6 °C Humidity: 33.5 %
After Pressure 100.96 kPa Temperature: 21.5 °C Humidity: 34.9 %

Test results summary


Test	Result
Linearity	Complies
Short Duration	Complies
Overload Latching	Complies
Frequency weighting	Complies
Absolute Acoustic Sensitivity	Complies

COPY

COPY

CERTIFICATE OF CALIBRATION

ISSUED BY Cirrus Research plc
DATE OF ISSUE 19 January 2024 CERTIFICATE NUMBER 206901



Cirrus Research plc
Acoustic House
Bridlington Road
Hunmanby
North Yorkshire
YO14 0PH
United Kingdom

Page 1 of 2
Approved signatory
N.Smith
Electronically signed:

N.D. Smith

Dosimeter : IEC 61252-1993+A1:2000

Instrument information

Manufacturer: Cirrus Research plc Notes: Eastern Thai Consulting 1992 Co.,Ltd.
Model: CR:110A 683 Moo.11, Sukaphibai 8 Rd., Nongkham,
Serial number: CA8879 Sriracha, Chonburi 20230
Firmware version: 5.4

Test summary

Date of calibration: 19 January 2024
The calibration was performed respecting the requirements of ISO/IEC 17025:2017.
The dosimeter submitted for testing successfully completed the periodic tests of IEC 61252-1993+A1:2000.
The dosimeter submitted for testing conforms to the specifications in IEC 61252-1993+A1:2000.

Test equipment

Equipment	Manufacturer	Model	Serial number
Signal Generator	SIGLENT	SDG 1032X	SDG1XDDQ6R6309
Attenuator	Cirrus Research	ZE:952	93892
Environmental Monitor	Cornel	T7510	16966334
doseBadge Reader	Cirrus Research plc	RC:110A	40088

Notes

This certificate provides traceability of measurement to the SI system of units and/or to units of measurement realised at the National Physical Laboratory or other recognised national metrology institutes. This certificate may not be reproduced other than in full except with the prior written approval of the issuing laboratory. The results within this certificate relate only to the items calibrated. The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor k=2, providing a coverage probability of approximately 95%.

CERTIFICATE OF CALIBRATION

Certificate Number:
206901

Page 2 of 2

Environmental conditions

The following conditions were recorded at the time of the test:

Before Pressure: 100.92 kPa Temperature: 21.6 °C Humidity: 35.3 %
After Pressure: 100.93 kPa Temperature: 21.7 °C Humidity: 40.1 %

Test results summary

Test	Result
Linearity	Complies
Short Duration	Complies
Overload Latching	Complies
Frequency weighting	Complies
Absolute Acoustic Sensitivity	Complies

COPY

COPY

CERTIFICATE OF CALIBRATION

ISSUED BY


Cirrus Research plc

DATE OF ISSUE

19 January 2024

CERTIFICATE NUMBER

206869



Cirrus Research plc
Acoustic House
Bridlington Road
Hummanby
North Yorkshire
YO14 0PH
United Kingdom

Page 1 of 2

Approved signatory

N Smith

Electronically signed:

Dosimeter : IEC 61252-1993+A1:2000

Instrument information

Manufacturer:

Cirrus Research plc

Notes:

Eastern Thai Consulting 1992 Co.,Ltd.
683 Moo.11, Sukaphibai 8 Rd., Nongkham,
Sriracha, Chonburi 20230

Model:

CR-110A

Serial number:

CA8886

Firmware version:

5.4

Test summary

Date of calibration: 19 January 2024

The calibration was performed respecting the requirements of ISO/IEC 17025:2017.

The dosimeter submitted for testing successfully completed the periodic tests of IEC 61252-1993+A1:2000.

The dosimeter submitted for testing conforms to the specifications in IEC 61252-1993+A1:2000.

Test equipment

Equipment	Manufacturer	Model	Serial number
Signal Generator	SIGLENT	SDG 1032X	SDG1XDDO6R6309
Attenuator	Cirrus Research	ZE:952	93892
Environmental Monitor	Comet	T7510	16966334
doseBadge Reader	Cirrus Research plc	RC:110A	40088

Notes

This certificate provides traceability of measurement to the SI system of units and/or to units of measurement realised at the National Physical Laboratory or other recognised national metrology institutes. This certificate may not be reproduced other than in full, except with the prior written approval of the issuing laboratory. The results within this certificate relate only to the items calibrated. The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor k=2, providing a coverage probability of approximately 95%.

CERTIFICATE OF CALIBRATION

Certificate Number:

206869

Page 2 of 2

Environmental conditions

The following conditions were recorded at the time of the test:

Before

Pressure:

100.96 kPa

Temperature:

21.5 °C

Humidity:

35.2 %

After

Pressure:

100.96 kPa

Temperature:

21.6 °C

Humidity:

33.4 %

Test results summary

Test	Result
Linearity	Complies
Short Duration	Complies
Overload Latching	Complies
Frequency weighting	Complies
Absolute Acoustic Sensitivity	Complies

COPY


COPY

CERTIFICATE OF CALIBRATION

ISSUED BY
Cirrus Research plc

DATE OF ISSUE
19 January 2024

CERTIFICATE NUMBER
206880



Cirrus Research plc
Acoustic House
Bridlington Road
Hunmanby
North Yorkshire
YO14 0PH
United Kingdom

Page 1 of 2

Approved signatory
N Smith
Electronically signed

Dosimeter : IEC 61252-1993+A1:2000

Instrument information

Manufacturer: Cirrus Research plc
Model: CR:110A
Serial number: CA8888
Firmware version: 5.4

Notes: Eastern Thai Consulting 1992 Co., Ltd.
683 Moo 11, Sukaphibai 8 Rd., Nongkhham,
Siracha, Chonburi 20230

Test summary

Date of calibration: 19 January 2024

The calibration was performed respecting the requirements of ISO/IEC 17025:2017.

The dosimeter submitted for testing successfully completed the periodic tests of IEC 61252-1993+A1:2000.

The dosimeter submitted for testing conforms to the specifications in IEC 61252-1993+A1:2000.

Test equipment

Equipment	Manufacturer	Model	Serial number
Signal Generator	KEYSIGHT	33511B	MY58001553
Attenuator	Cirrus Research	ZE:952	78713
Environmental Monitor	Comet	T7510	16966334
doseBadge Reader	Cirrus Research plc	RC:110A	100498

Notes

This certificate provides traceability of measurement to the SI system of units and/or to units of measurement realised at the National Physical Laboratory or other recognised national metrology institutes. This certificate may not be reproduced other than in full, except with the prior written approval of the issuing laboratory. The results within this certificate relate only to the items calibrated. The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor $k=2$, providing a coverage probability of approximately 95%.

CERTIFICATE OF CALIBRATION

Certificate Number:
206880

Page 2 of 2

Environmental conditions

The following conditions were recorded at the time of the test:

Before Pressure: 100.93 kPa Temperature: 21.4 °C Humidity: 34.6 %
After Pressure: 100.92 kPa Temperature: 21.6 °C Humidity: 35.3 %

Test results summary

Test	Result
Linearity	Complies
Short Duration	Complies
Overload Latching	Complies
Frequency weighting	Complies
Absolute Acoustic Sensitivity	Complies

COPY

COPY

CERTIFICATE OF CALIBRATION

ISSUED BY

Cirrus Research plc

DATE OF ISSUE

19 January 2024

CERTIFICATE NUMBER

206920

CERTIFICATE OF CALIBRATION

Certificate Number:
206920

Page 2 of 2

Environmental conditions

The following conditions were recorded at the time of the test:

Before

Pressure: 100.02 kPa

Temperature: 21.9 °C

Humidity: 34.6 %

After

Pressure: 100.03 kPa

Temperature: 21.8 °C

Humidity: 36.1 %



Cirrus Research plc

Acoustic House

Bridlington Road

Hunmanby

North Yorkshire

YO14 0PH

United Kingdom

Page 1 of 2

Approved signatory

N Smith

Electronically signed:



Dosimeter : IEC 61252-1993+A1:2000

Instrument information

Manufacturer:

Cirrus Research plc

Model:

CR:110A

Serial number:

CB0642

Firmware version:

5.4

Notes:

Eastern Thai Consulting 1992 Co.,Ltd.
683 Moo 11, Sukaphibai 8 Rd., Nongkham,
Sriracha, Chonburi 20230

Test summary

Date of calibration:

19 January 2024

The calibration was performed respecting the requirements of ISO/IEC 17025:2017.

The dosimeter submitted for testing successfully completed the periodic tests of IEC 61252-1993+A1:2000.

The dosimeter submitted for testing conforms to the specifications in IEC 61252-1993+A1:2000.

Test equipment

Equipment	Manufacturer	Model	Serial number
Signal Generator	KEYSIGHT	33511B	MY58001553
Attenuator	Cirrus Research	ZE:952	78713
Environmental Monitor	Comet	T7510	16966334
doseBadge Reader	Cirrus Research plc	RC:110A	100498

Notes

This certificate provides traceability of measurement to the SI system of units and/or to units of measurement realised at the National Physical Laboratory or other recognised national metrology institutes. This certificate may not be reproduced other than in full, except with the prior written approval of the issuing laboratory. The results within this certificate relate only to the items calibrated. The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor k=2, providing a coverage probability of approximately 95%.

COPY

COPY

CERTIFICATE OF CALIBRATION

ISSUED BY Cirrus Research plc
DATE OF ISSUE 19 January 2024 CERTIFICATE NUMBER 206879



Cirrus Research plc
Acoustic House
Bridlington Road
Hummerby
North Yorkshire
YO14 0PH
United Kingdom

Page 1 of 2
Approved signatory
N.Smith
Electronically signed:

Dosimeter : IEC 61252-1993+A1:2000

Instrument information

Manufacturer: Cirrus Research plc Notes: Eastern Thai Consulting 1992 Co.,Ltd.
Model: CR:110A 683 Moo.11, Sukaphibai 8 Rd., Nongkham,
Serial number: CB0640 Sriracha, Chonburi 20230
Firmware version: 5.4

Test summary

Date of calibration: 19 January 2024
The calibration was performed respecting the requirements of ISO/IEC 17025:2017.
The dosimeter submitted for testing successfully completed the periodic tests of IEC 61252-1993+A1:2000.
The dosimeter submitted for testing conforms to the specifications in IEC 61252-1993+A1:2000.

Test equipment

Equipment	Manufacturer	Model	Serial number
Signal Generator	KEYSIGHT	33511B	MY58001553
Attenuator	Cirrus Research	ZE-952	78713
Environmental Monitor	Comet	T7510	16966334
doseBadge Reader	Cirrus Research plc	RC:110A	100498

Notes

This certificate provides traceability of measurement to the SI system of units and/or to units of measurement realised at the National Physical Laboratory or other recognised national metrology institutes. This certificate may not be reproduced other than in full, except with the prior written approval of the issuing laboratory. The results within this certificate relate only to the items calibrated. The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor k=2, providing a coverage probability of approximately 95%.

CERTIFICATE OF CALIBRATION

Environmental conditions

The following conditions were recorded at the time of the test:

Before Pressure: 99.84 kPa Temperature: 21.4 °C Humidity 32.5 %
After Pressure: 99.87 kPa Temperature: 21.7 °C Humidity: 33.5 %

Test results summary

Test	Result
Linearity	Complies
Short Duration	Complies
Overload Latching	Complies
Frequency weighting	Complies
Absolute Acoustic Sensitivity	Complies

COPY

COPY



Certificate No. : 23-148799
Sample Code : 23-56200-001

CERTIFICATE OF CALIBRATION

Customer : EASTERN THAI CONSULTING 1992 CO., LTD.
683 Moo 11, Sukhapibarn 8 Rd., Nongkham,
Sriracha, Chonburi 20230

Location of Calibration : EASTERN THAI CONSULTING 1992 CO., LTD.
(Analytical Balance Room)

Equipment : ELECTRONIC BALANCE

Manufacturer : METTLER TOLEDO

Model : XS205DU

Serial No. : 1126323724

ID No. : LABE 05/1

Date of Receipt : 22 December 2023

Date of Calibration : 22 December 2023

Calibrated by : Mr. Somwang Sangdee
Scientist
Approved by : (Mr. Somchai Neampunt)
Signed for Director

Issue date : 25 December 2023

The uncertainties are for a confidence probability of approximately 95%.

The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Asia Medical and Agricultural Laboratory and Research Center Public Company Limited (AMARC).



Certificate No. : 23-148799
Sample Code : 23-56200-001

REPORT OF CALIBRATION

Equipment : ELECTRONIC BALANCE
Manufacturer : METTLER TOLEDO
Model : XS205DU
Capacity : Max 81 g / 220 g
Resolution : 0.01 mg / 0.1 mg
Serial No. : 1126323724
ID No. : LABE 05/1

Result of Calibration

1. Test weight and repeatability of reading

Repeatability is a measure of the ability of a balance to supply the same result in repetitive weighings with one and the same load under the same measurement condition. The measurement of the repeatability must include both the balance specifications and the ambient (vibration, fluctuating air current/temperature/humidity, etc.) Operator handling of the balance is also included in the standard deviation.

Unit : g	Range : 80	Before adjustment	After adjustment
<input type="checkbox"/> No adjustment	Nominal value	40 80 40 80	
<input checked="" type="checkbox"/> Adjustment	Standard weight	40.000054 80.000048 40.000054 80.000048	
	Average reading of indicator	40.000026 80.000037 40.000017 80.000017	
	Standard deviation	0.000015 0.000016 0.000008 0.000009	

Unit : g	Range : 200	Before adjustment	After adjustment
<input type="checkbox"/> No adjustment	Nominal value	100 200 100 200	
<input checked="" type="checkbox"/> Adjustment	Standard weight	100.000042 200.000041 100.000042 200.000041	
	Average reading of indicator	100.00003 200.00004 100.00001 200.00001	
	Standard deviation	0.000005 0.000005 0.000003 0.000005	





Certificate No. : 23-148799

Sample Code : 23-56200-001

REPORT OF CALIBRATION

Result of Calibration

2. Sensitivity or value of a scale division

Change in the output variable of a measuring instrument divided by the associated change in the input variable.

Unit : g

Range : 80		Range : 200	
Test Point	Sensitivity, S	Test Point	Sensitivity, S
0	1.00748	0	1.0274
40	0.98753	100	0.9975
80	0.99751	200	0.9975

3. Departure of indication from nominal value, Linearity

Unit : g

Nominal Value	Standard Value	Average Reading of Indicator	Correction Value	Expanded Uncertainty	Coverage Factor (k)
Unload	0.0000000	0.00000	0.00000	0.000012	2.05
0.01	0.0100025	0.01000	0.00000	0.000012	2.05
0.1	0.1000019	0.10001	-0.00001	0.000013	2.03
1	1.0000125	1.00001	0.00000	0.000015	2.02
5	5.0000208	5.00004	-0.00002	0.000021	2.00
10	10.0000004	10.00008	-0.00008	0.000026	2.00
20	20.0000030	20.00011	-0.00008	0.000036	2.00
50	50.000014	50.00014	-0.00013	0.000088	2.00
100	100.000042	100.0001	-0.0001	0.00016	2.00
150	150.000056	150.0001	0.0000	0.00022	2.00
200	200.000041	200.0002	-0.0002	0.00027	2.00

The result expanded uncertainty of measurement U is stated as the standard uncertainty of measurement multiplied by the coverage factor k , which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty of measurement has been determined in accordance with UKAS M3003.

COPY

fumi



Certificate No. : 23-148799

Sample Code : 23-56200-001


REPORT OF CALIBRATION

Result of Calibration :

4. Eccentric or off-centre loading

Deviation of the measurement value through off-center (eccentric) loading. The corner load increases with the weight of the load and its removal from the center of the pan support.

Weighing pan		Test weight : 50 and 100	
		Unit : g	
Range	Position	Reading of indicator	Reading of indicator
80	1	50.00015	100.0001
	2	50.00022	100.0001
	3	50.00008	100.0001
	4	50.00002	100.0000
	5	50.00016	100.0002
	6	50.00014	100.0001
Maximum difference		0.00013	0.0001

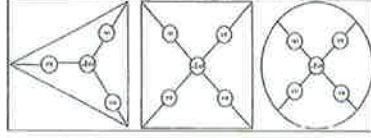

Condition of Calibration

Calibration Method : W1-C1-004 base on UKAS LAB 14: 2019		Ambient conditions	
		Min	Max
2. This result of calibration was found accurate as shown on date and place of calibration only.		Temperature (°C)	22.8 23.0
3. Condition of Calibration tem: Normal		Relative Humidity (%Rh)	43.5 51.1
4. This certification is traceable to the International System of Unit maintained at : Through the reference standard laboratory of Asia Medical and Agricultural Laboratory and Research Center Public Company Limited (instrument number 1).		Air pressure (hPa)	1012.5 1014.5

5. Reference standard instrument :

Instrument

1) STANDARD WEIGHT 1 kg to 1 kg

Class

ID No.

E2 LB-WE-79

Certificate No.

23-105642

Due Date

10 September 2024


End of Report

COPY

fumi

PinAAcle 900F Preventive Maintenance (PM)

Company Name:	Eastern Thai Consulting 1992 Co., Ltd.		
Address (Instrument Location):	683 Moo 11 Sukapibal 8 Rd. Nong Kham, Si Racha, Chonburi 20230		
Serial Number:	PFBS22080801	PM Number:	2 of 2
Customer Name (if applicable):		Telephone Number:	
Customer Support Engineer Name:	Khwanchai	Service Order Number:	WO-01886639
Date PM Performed: (DD-MM-YY)	24-Oct-2023	Next PM Due Date: (DD-MM-YY)	24-Apr-2024
Standard Labor Hours to Complete PM :		5 hours	

Part Number	Release	Publication Date	 PerkinElmer®
09370145 Rev.9	A	January 2018	

Scope

The purpose of this PM is to ensure the continued functionality of the PinAAcle 900F by inspecting and replacing any worn or damaged parts. This service should only be performed by a trained representative of PerkinElmer.

The customer should save their method before the PM begins.

General Instructions:

The customer must provide the engineer operational data to demonstrate recent instrument performance prior to starting the PM.

Always check with the customer before making any changes that may affect the customer's analysis or calibration, including a current back-up of system software and/or data files.

The completed document should be signed by an authorized PerkinElmer and customer representative and left with the customer.

Update the PM sticker and instrument logbook as required.

Copyright Information

This document contains proprietary information that is protected by copyright. All rights are reserved.

No part of this publication may be reproduced in any form whatsoever or translated into any language without the prior, written permission of PerkinElmer, Inc.

Copyright © 2013 PerkinElmer, Inc.

Trademarks

Registered names, trademarks, etc. used in this document, even when not specifically marked as such, are protected by law. PerkinElmer is a registered trademark of PerkinElmer, Inc. All other trademarks and registered trademarks not owned by PerkinElmer Inc. or its subsidiaries that are depicted herein are the property of their respective owners. Except as specifically set forth in its terms and conditions of sale, PerkinElmer makes no Warranty of any kind with regard to this document, including, but not limited to, the implied warranties of merchantability and fitness for a particular purpose.

PerkinElmer shall not be liable for incidental or consequential damages in connection with the furnishing or use of this document.

Component List

Component / Specific Model	Serial #	Configuration Notes
FIAS100		

Parts Lists

Parts Included with the PM		
Part Number (if applicable)	Description	Quantity
80501696	Fan Filters	NA
N3160156	O-Ring Kits for Sampling Introduction (Stainless Steels Nebulizer)	NA
N3160157	O-Ring Kits for Sampling Introduction (Plastic Nebulizer)	NA
N9301714	Replacement Acetylene Filter Cartridge	NA
TH001022	Replacement Air Filter Cartridge	NA

Additional Reagents and Standards Required for PM

Part Number (if applicable)	Description	Quality	Batch/Lot #	Expired Date (MM/YY)
N9300183	1000 mg/L Copper Standard	AR	26-87/CLY1	30-Jan-2024

Additional Reagents and Standards Required for PM (Customer Support Solution)

Part Number (if applicable)	Description	Quantity	Batch/Lot #	Expiration Date (MM/YY)
N/A	DI Water	250 ml.	AR	AR
N/A	0.5% HNO ₃	250 ml.	AR	AR

COPY

COPY

Additional Tools Required for PM

Part Number (if applicable)	Description	Quantity	Serial #
N1013000	0.2A Neutral density filter	1	MG0-056
N1013002	1.0A Neutral density filter	1	MG2-054
03030997	System 2 EDL Driver	1	03030997
N3050605	As System 2 EDL	1	16148
N3050121	Cu Lumina HCL	1	092216-010130
N3050109	Ba Lumina HCL	1	102416-040160
N3050139	K Lumina HCL	1	110716-010060
N3050152	Ni Lumina HCL	1	100516-030190

Procedure Checklist

Use (✓) to check off those steps in the checklist that have been completed.

1. General:

- ☒ Review the instrument performance with the customer and document any recent problems.
- ☒ Inspect the customer log book and make any appropriate PM entries.
- ☒ Perform general inspection of system for cleanliness.

2. PC Instrument Software:

- ☒ Instrument Software user files/databases archived, packed, and/or deleted as needed.

3. Mechanical:

- ☒ Inspect and clean all fans and filters. Replace filters if necessary
- ☒ Inspect all gas lines for leaks and/or wear. Replace if needed.
- ☒ Clean exterior of the instrument.
- ☒ Inspect the burner head, burner chamber, and nebulizer. Clean if needed as stated in the Hardware Guide.
- ☒ Check burner head dimensions with the feeler gauge as stated in the Hardware Guide in the Maintenance chapter section on cleaning the burner head and checking sloth width. Replace if out of specification
- ☒ Check the condition of the end cap, burner head, and nebulizer O-rings. Replace if necessary.
- ☒ Check the drain system for signs of wear. Replace worn or damaged parts.
- ☒ Visually check for proper flame conditions when igniting the Air-C2H2 and N2O-C2H2 flames (if applicable).

4. Electrical:

- ☒ Inspect PC boards. Clean if necessary.
- ☒ Carefully check all internal and external cable connections.
- ☒ Check instrument firmware revisions upgrade to current levels (if necessary)
- ☒ Run Diagnostics Test within the Advanced function of the Spectrometer page. Check the results in the service log folder in the Spectrometer BM Log Viewer.

5. Optics:

- ☒ Inspect and clean the sample compartment windows, if needed.
- ☒ Inspect optics. Clean or replace if necessary.

6. Gasses:

- ☒ Verify that the Gasses supplied to the instrument are within the pressure and purity specifications found in the PinAAcle 900 Series Pre-installation Checklist SDB.
- ☒ Verify that the acetylene filter and air filter element is dry. Replace if necessary.

7. Flame Interlock Check:

Description: Check to ensure that all safety interlocks are closed.

Parameter	Specification	Test Results	Pass/Fail
Flame Sensor	Air/C ₂ H ₂ Flame correctly shuts down	Active	Pass
Drain Sensor	Air/C ₂ H ₂ Flame correctly shuts down	Active	Pass
Nebulizer Sensor	Air/C ₂ H ₂ Flame correctly shuts down	Active	Pass
C ₂ H ₂ Pressure Sensor	Air/C ₂ H ₂ Flame correctly shuts down	Active	Pass
Air Pressure Sensor	Air/C ₂ H ₂ Flame correctly shuts down	Active	Pass
Burner Head Sensor	Choosing Nitrous Oxide as the oxidant should trigger an interlock shuts down	Active	Pass

8. After PM Performance tests:

8.1 Detector Linearity with Barium

Description: Ensures that the detector is linear in the Visible Range.

Parameter	Specification	Certificate Value at 553.6 nm (Abs.)	Test Results	Pass/Fail
1.0 A ND Filter	±5% from Cert.	1.0531	1.0230	Pass
0.2 A ND Filter	±5% from Cert.	0.1806	0.1783	Pass

8.2 Baseline Noise at 1.0 Absorbance with Barium

Description: Ensures that a high absorbance will not produce excessive noise.

Parameter	Specification	Results	Pass/Fail
Standard Deviation	≤0.010	0.0015	Pass

8.3 AA Baseline Noise with Copper

Description: Check baseline noise.

Parameter	Specification	Results	Pass/Fail
Standard Deviation	≤0.001	0.0001	Pass

8.4 D₂ Background Compensation with Copper

Description: Verifies the instruments ability to compensate for Background absorption.

Parameter	Specification	Results	Pass/Fail
Standard Deviation	≤0.010	0.0054	Pass

8.5 AA-BG Baseline Noise with Copper

Description: Ensures that background correction does not produce excessive noise.

Parameter	Specification	Results	Pass/Fail
Standard Deviation	≤0.005	0.0001	Pass

8.6 AA-BG Baseline Noise with Arsenic

Description: Ensures that background correction does not produce excessive noise at a low wavelength.

Parameter	Specification	Results	Pass/Fail
Standard Deviation	≤0.005	0.0002	Pass

8.7 Flame Sensitivity

Description: Instrument Sensitivity checked against Copper standard.

Standard Copper Sensitivity	Specification	Results (Abs.)	Pass/Fail
5 mg/L Sensitivity S5 Neb (if applicable)	> 0.250 Abs.	NA	NA
2 mg/L Sensitivity HS Neb (if applicable)	> 0.250 Abs.	0.3878	Pass

10. Review:

- ☒ Review with the customer PM work performed.
- ☒ Review with the customer routine maintenance procedures.
- ☒ Discuss recommended customer supplied materials to have on hand.
- ☒ Attach PM sticker.

COPY

COPY

Additional Comments

Additional Comments Regarding the PM

Review

The preventive maintenance checks and if applicable performance tests for PinAAcle 900F have been completed.

This PinAAcle 900F Passes ☒ Fails ☐ the preventive maintenance.

Review of Preventive Maintenance:

Authorized PerkinElmer Representative:	KL S.	Date:	24-Oct-2023 (DD-MM-YY)
Authorized Customer Representative:	001025206	Date:	24-Oct-2023 (DD-MM-YY)

Handwritten
COPY



Certificate No. : 23-148800

Sample Code : 23-56200-002

CERTIFICATE OF CALIBRATION

Customer : EASTERN THAI CONSULTING 1992 CO., LTD.
683 Moo 11, Sukhapibarn 8 Rd., Nongkham,
Sriacha, Chonburi 20230

Location of Calibration : EASTERN THAI CONSULTING 1992 CO., LTD.
(Analytical Balance Room)

Equipment : ELECTRONIC BALANCE

Manufacturer : SARTORIUS

Model : SECURA224-1S

Serial No. : 0036707137

ID No. : LABE 05/2

Date of Receipt : 22 December 2023

Date of Calibration : 22 December 2023

Calibrated by Mr. Somwang Sangdee
Scientist

Issue date : 25 December 2023

The uncertainties are for a confidence probability of approximately 95%.

The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Asia Medical and Agricultural Laboratory and Research Center Public Company Limited (AMARC).



Certificate No. : 23-148800

Sample Code : 23-56200-002

REPORT OF CALIBRATION

Equipment : ELECTRONIC BALANCE
Manufacturer : SARTORIUS
Model : SECURA224-1S
Capacity : Max 220 g
Resolution : 0.0001 g
Serial No. : 0036707137
ID No. : LABE 05/2

Result of Calibration

1. Test weight and repeatability of reading

Repeatability is a measure of the ability of a balance to supply the same result in repetitive weighings with one and the same load under the same measurement condition. The measurement of the repeatability must include both the balance specifications and the ambient (vibration, fluctuating air current/temperature/humidity, etc.) Operator handling of the balance is also included in the standard deviation.

Unit : g	Range : 220	Before adjustment	After adjustment
<input type="checkbox"/> No adjustment	Nominal value	100 200 100 200	100 200
<input checked="" type="checkbox"/> Adjustment	Standard weight	100.000042 200.000041 100.000042 200.000041	100.000041 200.000041
	Average reading of indicator	99.9998 199.9998	100.0000 200.0000
	Standard deviation	0.00006 0.00007	0.00003 0.00007

Unit :	Range :	Before adjustment	After adjustment
<input type="checkbox"/> No adjustment	Nominal value	*	*
<input type="checkbox"/> Adjustment	Standard weight	*	*
	Average reading of indicator	*	*
	Standard deviation	*	*

COPY



Certificate No. : 23-148800

Sample Code : 23-56200-002

REPORT OF CALIBRATION

Result of Calibration

2. Sensitivity or value of a scale division

Change in the output variable of a measuring instrument divided by the associated change in the input variable.

Unit : g

Range : 220

Range :

Test Point	Sensitivity, S	Test Point	Sensitivity, S
0	0.7980	-	-
100	0.8978	-	-
200	0.8978	-	-

3. Departure of indication from nominal value, Linearity

Unit : g

Nominal Value	Standard Value	Average Reading of Indicator	Correction Value	Expanded Uncertainty	Coverage Factor (k)
Unload	0.0000000	0.0000	0.0000	0.000086	2.00
0.01	0.0100025	0.0100	0.0000	0.000086	2.00
0.1	0.1000019	0.1000	0.0000	0.000087	2.00
1	1.0000125	1.0000	0.0000	0.000087	2.00
2	2.0000089	2.0000	0.0000	0.000087	2.00
5	5.0000208	5.0001	-0.0001	0.000088	2.00
10	10.000004	10.0000	0.0000	0.000090	2.00
20	20.000030	20.0000	0.0000	0.000093	2.00
50	50.000014	50.0000	0.0000	0.00011	2.00
100	100.000042	100.0000	0.0000	0.00016	2.00
200	200.000041	200.0000	0.0000	0.00028	2.00

The result expanded uncertainty of measurement U is stated as the standard uncertainty of measurement multiplied by the coverage factor k, which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty of measurement has been determined in accordance with UKAS M3003.

COPY

fms



Certificate No. : 23-148800

Sample Code : 23-56200-002


REPORT OF CALIBRATION

Result of Calibration :

4. Eccentric or off-centre loading

Deviation of the measurement value through off - center (eccentric) loading. The corner load increases with the weight of the load and its removal from the center of the pan support.

Weighing pan		Test weight : 100
		Unit : g
		Range : 220
Position	Reading of indicator	Reading of indicator
1	100.0000	-
2	100.0000	-
3	100.0000	-
4	99.9999	-
5	100.0000	-
6	100.0000	-
Maximum difference	0.0001	-

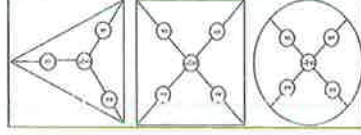

Condition of Calibration

1. Calibration Method : WI-CL-004 base on UKAS LAB 14: 2019
2. This result of calibration was found accurate as shown on date and place of calibration only.
3. Condition of Calibration item: Norma
4. This certification is traceable to the International System of Unit maintained at : *

Through the reference standard laboratory of Asia Medical and Agricultural Laboratory and Research Center Public

Company Limited (Instrument number : 1)

5. Reference standard instrument :

Instrument

- 1) STANDARD WEIGHT 1 mg to 1 kg

Class : E2

ID No. : LB-WF-79

Certificate No. : 23-105642

Due Date : 10 September 2024

End of Report -

COPY



MIRACLE INTERNATIONAL TECHNOLOGY CO., LTD
214 Bangwaek Rd. Bangnai Bangkok 10160
Tel.: 0-2865-4647-8 Fax: 0-2865-4649 <http://www.mit.in.th>



CALIBRATION CERTIFICATE

Customer

: Eastern Thai Consulting 1992 Co., Ltd.
683 Moo 11, Sukhapibarn 8 Rd., Nongkham, Sriracha, Chonburi 20230

Certificate No. : L202405022-0013
Date Issued : 08-May-24

Equipment

: Analog Barometer

Manufacturer

: Barigo

Model

: -

Serial No.

: -

ID No./Tag No.

: BM001/41

Date Received

: 03-May-24

Date Calibrated

: 06-May-24

Calibrated by

: Mr. Saruth Srichutikul

Calibration Method or Calibration Procedure Used

In-house method : CP-21 base on DKD-R 6-1: Edition 3 2014.

This certificate is traceable to national standards, which realize the units of measurement according to the International System of Units (SI).

Result of Calibration

The reported uncertainty of measurement was based on standard uncertainty multiplied by a coverage factor $k = 2$, providing a level confidence approximately 95 percent.

This certificate may not be reproduced other than in full except with the prior written approval of the Miracle International Technology Company Limited.

Approved by:

Sarayuth T.
(Mr. Sarayuth Tochua)

Page 1 of 2



COPY

Certificate No : L202405022-0013

Environment Ambient Temperature : (25 ± 2)°C

Relative Humidity : (50 ± 15)%RH

STD Reading mbar	UUC Reading (mbar) Before Adjusted	UUC Reading (mbar) After Adjusted	UUC Error mbar	Uncertainty ± mbar	MPE ± mbar	Pass with Guar
990.00	990	-	0.00	0.59	10.3	Pa
1000.00	1000	-	0.00	0.59	10.3	Pa
1010.00	1010	-	0.00	0.59	10.3	Pa
1020.00	1020	-	0.00	0.59	10.3	Pa
1030.00	1030	-	0.00	0.59	10.3	Pa

STD = Standard Pass = $|\text{error}| + |\text{uncertainty}| \leq |\text{MPE}|$

UUC = Unit Under Calibration Fail = $|\text{error}| + |\text{uncertainty}| > |\text{MPE}|$

MPE = Maximum Permissible Error

Calibrated condition :

Pressure Medium

Mounting Position

Reference Level

Conversion Factor

Air : Density = 1.19 kg/m³ @ 20°C. 1 bar

Vertical

at center of its dial

Multiply by 1.0 E+02 - Pa unit

Description of UUC :

Range

950 - 1080 mbar Absolute

Calibration Range

990 - 1030 mbar Absolute

Scale Interval

1 mbar

Condition As-Received : Used Item

The measurement results and statements of conformity with specification only relate to the item calibrated.

Measurement Standards Used & Traceability :

The International System of Units (SI) through


IRPC Certificate No. CL1-P230097 for Reference Pressure Monitor Serial No. 1598, Due 09-Nov-24

End of Certificate

COPY

SK

S K SALES AND SERVICE CO.,LTD.
194/56, 194/57 Thakham Rd. Samsae Dam
Bang Khun Thien Bangkok 10150
Tel : 02-417-2144 Fax : 02-417-2155



Certificate of Calibration

Reference No. : C03190/2309-025
Customer : Eastern Thai Consulting 1992 Co.,Ltd.
683 Moo 11, Sukhaphiban 8, Tambol Nongkham,
Siracha District, Chonburi 20230, Thailand

Equipment : Incubator
Manufacturer : Lovibond
Model : TC445S
Serial No. : 0223/007275
ID No. :
Received Date : 15 September 2023
Calibrated Date : 15 September 2023
Issued Date : 18 September 2023
Environment :

	Minimum Value	Maximum Value
Ambient Temperature (°C)	27.5	28.1
Relative Humidity (% RH)	57	58
AC Line Voltage (VAC)	224	226

Place Of Calibration : Production Line
Calibrated by : Mr. Teerasak Chalyaporn

Calibration Method

In-house method : SK-WI-23 base on Thai Laboratory Accreditation Scheme Publication Reference G-20

Condition of this result of calibration

- Reference standard instrument

Instrument	Serial No.	Certificate No.	Due Date
1) Data acquisition/Switch unit	MY44047397	L2305-268	4 November 2023
2) Multiplexer Module	MY41105123	L2305-268	4 November 2023
- This result of calibration was found accurate as shown on date and place of calibration only
- This certificate can be traceable to International System of Unit :

Through Thailand Institute of Scientific And Technological Research (TISTR)

Approved by

☒ Mr. Suphachai Saksi ☐ Mr. Phayak Toolit ☐ Miss Tantaraporn Petpong

The reported uncertainty is based on a standard uncertainty multiplied by a coverage factor $k = 2.0$, providing a level of confidence level of approximately 95 %

This certificate may not be reproduced other than in full except with the prior written approval of the S K Sales And Service Company Limited

COPY

Certificate No. : S2309-3014

Page 2 of 2

Table1 General Information

Working Area (W*L*H)	60 *56 *145 cm
Fresh Air	OFF

Table2 Chamber Performance


Setting Temperature (°C)	Average Indicating Temperature (°C)	Measured Stability (± °C)	Measured Uniformity (°C)	Overall Variation (°C)
20.0	20.0	0.37	0.64	0.98

Table3 Temperature Distribution

Setting Temperature (°C)	Average Standard Reading (°C)									Uncertainty (± °C)
	No. 1	No. 2	No. 3	No. 4	No. 5	No. 6	No. 7	No. 8	No. 9	
20.0	19.52	19.40	19.70	19.43	19.33	19.39	19.45	19.58	19.67	0.55

Resolution : 0.1 (°C)

* Probe No. 9 is Reference Probe



- Notes :
- The temperature stability is the one-half of greatest maximum difference of measured temperatures at any one probe.
 - The temperature uniformity is the maximum difference of measured temperatures between of any probes and the measured temperature at the reference location which are observed at same time
 - Overall variation is the difference of maximum and minimum measured temperatures throughout observation time.
 - The reported uncertainty of measurement were excluded Uniformity and Stability

** End of Calibration Report **

COPY

[Handwritten signature]

Results of Calibration

Resolution : 0.1 °C

1. Reporting of Temperature

Calibration point (°C)	UUC* setting (°C) reading (°C)	UUC*	Measured temperature at each positions (°C)										Uncertainty ± (°C)	Coverage factor k
			# 1	# 2	# 3	# 4	# 5	# 6	# 7	# 8	# 9 [±]			
20	20.5	20.0	20.28	19.86	19.90	19.91	19.82	20.10	20.01	19.89	19.75	0.59	2.00	

2. Characterization results

Calibration point (°C)	Stability ± (°C)	Uniformity (°C)	Overall variation (°C)
20	0.45	0.85	1.31

Notes

UUC* = Unit Under Calibration



REPORT OF CALIBRATION


Certificate No. : 24-046203

Sample Code : 24-18906-002

Results of Calibration

Notes

- Sensor installation locations
 - All sensors at any corners or walls should be positioned 5 cm (a x b x c) from the wall.
 - The reference sensor is preferably located of the geometric center of the chamber.
- Interior dimensions approx of chamber :
W = 60 cm ; D = 56 cm ; H = 146 cm
- Air valve or fresh air level : Off
- Fan level : Open
- The quoted uncertainty includes "Stability of chamber and loading effect in chamber at 20% of uniformity".
- Uniformity - the maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time.
- Stability - one-half of the greatest maximum difference of measured temperatures at any one sensor.
- Overall variation - the difference of the maximum and the minimum measured temperatures throughout observation time.
- UUC* reading - the average reading of indicating device that forms the integral part of the enclosure.
- Calibration results without adjustment.

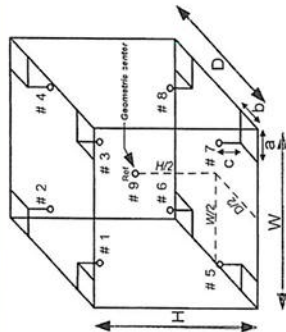Figure: Example of sensor
Installation Positions

The result expanded uncertainty of measurement U is stated as the standard uncertainty of measurement multiplied by the coverage factor k , which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty of measurement has been determined in accordance with UKAS M3003

- End of Report -

COPY

NSC-TSI-TS17025
CALIBRATION 0152

Page 1 of 3

Certificate No. : 24-001944

Sample Code : 24-00963-001

CERTIFICATE OF CALIBRATION

Customer : EASTERN THAI CONSULTING 1992 CO., LTD.
683 Moo 11, Sukhapibarn 8 Rd., Nongkham,
Sriracha, Chonburi 20230

Location of Calibration : EASTERN THAI CONSULTING 1992 CO., LTD.
(Hot Lab)

Equipment : Temperature controlled enclosures (Hot air oven)
Manufacturer : Memmert
Model : UM 400
Serial No. : 900982
ID No. : LABE 17/1
Date of Receipt : 09 January 2024
Date of Calibration : 09 January 2024

Condition of Calibration

1. Environment
1.1 Ambient temperature : Maximum 30.6 °C ; Minimum 29.2 °C
1.2 Relative humidity : Maximum 57.5 % ; Minimum 46.4 %
1.3 Line voltage supplied : Maximum 229.5 VAC ; Minimum 222.5 VAC

2. Calibration method

TLAS-G-20: Guidelines for calibration and checks of temperature controlled enclosures.

3. Reference standard instrument

Instrument	ID No.	Certificate No.	Due Date
Data Acquisition With Sensor (RTD-Pt100)	LB-DA-10 (RTD-257 to RTD-265)	23-066256	29 June 2024

4. This certificate is traceable to the international system of unit (SI Unit).

The measurement is traceable to Asia Medical and Agricultural Laboratory and Research Center Public Company Limited.

5. This result of calibration was found accurate as shown on date and place of calibration only.

6. Condition of calibration item : Normal

Calibrated by

Mr. Sarawoot Thammo

Approved by

(Mr. Somchai Neampunt)

Issue date

09 January 2024

The uncertainties are for a confidence probability of approximately 95%.

The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Asia Medical and Agricultural Laboratory and Research Center Public Company Limited (AMARC).

361 Soi Ladprao 122, Ladprao Road,

Phlabphla, Wang Thonglang, Bangkok 10310

FM CL 114

TEL 02-516-2422

FAX 02-516-6949

Rev 01

CONTACT@AMARC.CO.TH

WWW.AMARC.CO.TH

Effective Date: 15/10/21

NSC-TSI-TS17025
CALIBRATION 0152

Page 2 of 3

Certificate No. : 24-001944

Sample Code : 24-00963-001

REPORT OF CALIBRATION

Results of Calibration

Resolution : 0.1 °C

1. Reporting of Temperature

Calibration point (°C)	UUC* setting (°C)	UUC* reading (°C)	Measured temperature at each positions (°C)								Uncertainty ± (°C)	Coverage factor k
			# 1	# 2	# 3	# 4	# 5	# 6	# 7	# 8	# 9 ^{Rev}	
60	60.0	60.0	60.04	59.90	59.81	59.84	59.47	59.91	60.08	59.98	59.87	2.00
85	85.0	85.0	86.07	85.75	85.58	85.62	84.69	85.83	86.28	85.94	85.77	2.00

2. Characterization results

Calibration point (°C)	Stability ± (°C)	Uniformity (°C)	Overall variation (°C)
60	0.11	0.49	0.80
85	0.09	1.13	1.72

Notes

UUC* = Unit Under Calibration

COPY

361 Soi Ladprao 122, Ladprao Road,

Phlabphla, Wang Thonglang, Bangkok 10310

FM CL 108

TEL 02-516-2422

FAX 02-516-6949

Rev 09

CONTACT@AMARC.CO.TH

WWW.AMARC.CO.TH

Effective Date: 15/10/21

NSC-TISI-TIS17025
CALIBRATION 0152

REPORT OF CALIBRATION

Page 3 of 3


Certificate No. : 24-001944

Sample Code : 24-00963-001

Results of Calibration

Notes

1. Sensor installation locations
 - 1.1 All sensors at any corners or walls should be positioned 5 cm (a x b x c) from the wall.
 - 1.2 The reference sensor is preferably located of the geometric center of the chamber.
2. Interior dimensions approx of chamber :
W = 40 cm ; D = 28 cm ; H = 39 cm
3. Air valve or fresh air level : Off
4. Fan level : Open
5. The quoted uncertainty includes "Stability of chamber and loading effect in chamber at 20% of uniformity".
6. Uniformity - the maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time.
7. Stability - one-half of the greatest maximum difference of measured temperatures at any one sensor.
8. Overall variation - the difference of the maximum and the minimum measured temperatures throughout observation time.
9. UUC* reading - the average reading of indicating device that forms the integral part of the enclosure.
10. Calibration results without adjustment.

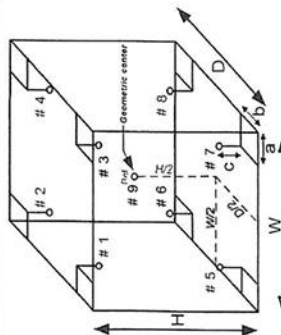Figure: Example of sensor
installation Positions

The result expanded uncertainty of measurement, U , is stated as the standard uncertainty of measurement multiplied by the coverage factor k , which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty of measurement has been determined in accordance with UKAS M3003.

- End of Report -

COPY



QUALITY CALIBRATION CO.,LTD.

235 Petchkasem 63/2 Road, Laksong, Bangkok, Bangkok 10160
Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584
www.qcalibration.com



CERTIFICATE No : 23T10864
REFERENCE No : 71117-1

PAGE : 1 OF 2

Certificate of Calibration

EQUIPMENT	: LIQUID IN GLASS THERMOMETER
MANUFACTURER	: PRECISION
MODEL	: 0 °C TO 100 °C
SERIAL No	: 43560
ID No	: LABE 16/1
RESOLUTION	: 0.1 °C
TYPE	: TOTAL IMMERSION
CONDITION AS RECEIVED	: USED ITEM
SUBMITTED BY	: EASTERN THAI CONSULTING 1992 CO., LTD. 683 MOO 11, SUKHAPIBAN 8 ROAD, NONGKHAM, SRIRACHA, CHONBURI 20230
CALIBRATED BY	: CHARUKIT L.
CALIBRATION DATE	: 09-Nov-23
APPROVED BY	: PONGSAK J.
ISSUED DATE	: 09-Nov-23
RECEIVED DATE	: 02-Nov-23

THIS CERTIFICATE MAY NOT BE REPRODUCED OTHER THAN IN FULL EXCEPT WITH THE PRIOR WRITTEN APPROVAL OF
QUALITY CALIBRATION CO., LTD.

COPY



QUALITY CALIBRATION CO.,LTD.

235 Petchkasem 63/2 Road, Laksong, Bangkok, Bangkok 10160
Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584
www.qcalibration.com

CERTIFICATE No : 23T10864

PAGE : 2 OF 2

Calibration Report

EQUIPMENT	: LIQUID IN GLASS THERMOMETER
MANUFACTURER	: PRECISION
MODEL	: 0 °C TO 100 °C
ID No	: LABE 16/1
RESOLUTION	: 0.1 °C
RECEIVED DATE	: 02-Nov-23
AMBIENT TEMPERATURE	: 23 °C ± 3 °C
SERIAL NUMBER	: 43560
TYPE	: TOTAL IMMERSION
CALIBRATION DATE	: 09-Nov-23
RELATIVE HUMIDITY	: 50 %RH ± 20 %RH

CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED BASED ON ASTM E77:1992 BY COMPARISON WITH STANDARD PLATINUM RESISTANCE THERMOMETER (SPRT) INTO LIQUID BATH TEMPERATURE CONTROLLER. THE TEMPERATURE SCALE USED WAS BASED ON ITS-90.

2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) STANDARD THERMOMETER	1502	77964	23T3927	08-Mar-24
2) SPRT PROBE	5614	636636	23T3927	08-Mar-24
3) PRECISION BATH	7320	A21105	22T13199	14-Dec-23
4) PRECISION BATH	CTR-40	A68155	22T13198	09-Dec-23
5) PRECISION BATH	6045	3C023	22T13200	19-Dec-23

3. THE CERTIFICATE IS VALID FOR THE ITEM CALIBRATED AS SHOWN ON THE DATE AND PLACE OF CALIBRATION ONLY.

4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.

5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-

- NATIONAL INSTITUTE OF METROLOGY (THAILAND).

RESULT OF CALIBRATION : WITHOUT ADJUSTMENT

STANDARD READING (°C)	UUC* READING (°C)	IMMERSION DEPTH (mm)	CORRECTION (°C)	EMERGENT STEM TEMPERATURE (°C)	UNCERTAINTY OF MEASUREMENT (±°C)
0.009	0.0	60	0.0090	N/A	0.26
25.01	25.0	165	0.0050	N/A	0.26
50.00	50.0	275	0.0040	N/A	0.26
99.991	100.0	360	-0.009	29.3	0.26

UUC* : UNIT UNDER CALIBRATION

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR k=2, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT

COPY

NSC-TIS-1517025
CALIBRATION0152

CERTIFICATE OF CALIBRATION

Page 1 of 3

Supersedes to Calibration Certificate No. 24-001949

Certificate No. : 24-001949/1

Sample Code : 24-00963-006

Customer : EASTERN THAI CONSULTING 1992 CO., LTD.
683 Moo 11, Sukhapibarn 8 Rd., Nongkham,
Sriracha, Chonburi 20230

Location of Calibration : EASTERN THAI CONSULTING 1992 CO., LTD.
(Laboratory)

Equipment : pH Meter
Manufacturer : METTLER TOLEDO
Serial No. : B448305208
Model : SevenCompact S220
ID No. : LABE 11/4
Date of Receipt : 09 January 2024
Date of Calibration : 09 January 2024

Condition of Calibration

1. Environment
1.1 Ambient temperature : 22.4 ± 0.2 °C 1.2 Relative humidity : 56.4 % ± 2.1 %

2. Calibration method
In house method WI-CL-019; based on direct measurement by using standard voltage calibrator and using certified reference material (CRM).

3. Reference standard / Certified reference material

Instrument	ID No.	Certificate No.	Due Date
3.1 Voltage Calibrator	LB-AMC-01	23E3244	03 October 2024
3.2 Digital Thermometer	LB-TH-33	23-098974	25 August 2024
Certified Reference Material	Lot No.	Ref No.	Expire Date
3.3 Buffer Solution pH 4.008	919273	PH216.L5	24 September 2025
3.4 Buffer Solution pH 6.886	941727	PH107.L5	06 November 2024
3.5 Buffer Solution pH 9.997	919278	PH220.L5	24 September 2024

4. This certificate is traceable to the international system of unit (SI Unit).

4.1 Instrument No. 3.1 through Technology Promotion Association (Thailand-Japan).
4.2 Instrument No. 3.2 through Asia Medical and Agricultural Laboratory and Research Center Public Company Limited.
4.3 Buffer Solution No. 3.3 and No. 3.5 traceable to CPA chem (through primary measurement method-Harned cell using calibrated thermometer, barometer, and nanovoltmeter Accredited laboratory ISO/IEC 17025 and ISO/IEC 17034).
4.4 Buffer Solution No. 3.4 traceable to CPA chem (CPA ReIN HARNED CELL LoIN 61275737; CPA ReIN HARNED CELL LoIN 61273986 Accredited laboratory ISO/IEC 17025 and ISO/IEC 17034).

5. This result of calibration was found accurate as shown on date and place of calibration only.

6. Condition of calibration item : Normal

Calibrated by Mr. Nuttaput Timula Approved by (Mr. Somchai Neampunt)

Issue date 31 January 2024
The uncertainties are for a confidence probability of approximately 95%.
The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of this laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Asia Medical and Agricultural Laboratory and Research Center Public Company Limited (AMARC).

NSC-TIS-1517025
CALIBRATION0152

REPORT OF CALIBRATION

Page 2 of 3

Supersedes to Calibration Certificate No. 24-001949

Certificate No. : 24-001949/1

Sample Code : 24-00963-006

Equipment : pH Meter
Manufacturer : METTLER TOLEDO
Serial No. : B448305208
Model : SevenCompact S220
ID No. : LABE 11/4
Range : -2,000 pH to 20,000 pH ; ±2000.0 mV ; -5.0°C to 130.0°C

Results of Calibration

Part 1. DC Voltage measurement
pH Meter Serial No. : B448305208

Nominal Value	Applied DC Voltage mV	Average indicator reading		Uncertainty mV	Coverage factor k
		mV	pH		
0	414.113	413.9	0.00	± 0.083	2.00
4	177.477	177.4	4.00	± 0.083	2.00
7	0.000	0.1	7.00	± 0.083	2.00
10	-177.477	-177.3	10.00	± 0.083	2.00
14	-414.113	-413.8	14.00	± 0.083	2.00

Part 2. Performance of Electrode system

Electrode Manufacturer : METTLER TOLEDO Model : InLab Expert Pro-ISM

Electrode Serial No. : 2453982

Three-Point Calibration at pH4, pH7 and pH10 Percent Slope : 98.3

Standard Buffer Solution pH (@ 25 °C)	Average indicator reading		Error Value pH	Uncertainty pH	Coverage factor k
	pH	mV			
4.008	4.01	182.1	0.002	± 0.010	2.00
6.886	7.00	7.8	0.014	± 0.011	2.00
9.997	10.01	-167.2	0.013	± 0.011	2.00

The result expanded uncertainty of measurement U is stated as the standard uncertainty of measurement multiplied by the coverage factor k , which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty of measurement has been determined in accordance with UKAS M3003.

COPY



REPORT OF CALIBRATION

Page 3 of 3

Supersede to Calibration Certificate No. 24-001949

Certificate No. : 24-001949/1

Sample Code : 24-00963-006

Equipment : pH Meter (Digital Thermometer with sensor)

Thermometer readout

Manufacturer : METTLER TOLEDO Model : SevenCompact S220

Serial No. : B44B305208 ID No. : LABE 11/4

Resolution : 0.1 °C Range : -5.0 °C to 130.0 °C

Thermometer sensor

Manufacturer : METTLER TOLEDO Model : InLab Expert Pro-ISM

Serial No. : 2453982 ID No. : N/A

Condition of Calibration

1. Environment
- 1.1 Ambient temperature : 22.6 °C ± 0.1 °C
- 1.2 Relative humidity : 55.1 % ± 3.3 %

2. Calibration method

- 2.1 The calibration use in house method WI-CL-021 : by comparison with standard thermometer
- 2.2 The calibration by comparison unit under calibration (UUC) to the standard thermometer in a calibration bath at the controlled temperature.
- 2.3 The temperature scale in use of this laboratory is the international temperature scale of 1990 (ITS-90).

3. Reference standard instrument

Instrument	Model	ID. No.	Certificate No.	Due date
3.1 Resistance Thermometer	PT-100	RTD-90	23-098974	25 August 2024
3.2 Thermometer Readout	GT-11	LB-TH-33	23-098974	25 August 2024

4. This certificate is traceable to the international system of unit (SI Unit).

Asia Medical and Agricultural Laboratory and Research Center Public Company Limited (Accreditation Under TLAS Laboratory Calibration No.0152)

5. This result of calibration was found accurate as shown on date and place of calibration only.

6. Condition of Calibration item : Normal

Results of Calibration

Calibration point °C	Average of standard reading °C	Unit under calibration		Expanded uncertainty °C	Coverage factor k
		Immersion depth mm	Average reading °C		
25	25.000	120	25.0	± 0.14	2.00

Notes

- Calibration results without adjustment

The result expanded uncertainty of measurement U is stated as the standard uncertainty of measurement multiplied by the coverage factor k , which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty of measurement has been determined in accordance with UKAS M0003

- End of report -

COPY



Certificate No. : 22-052238
Sample Code : 22-19150-003

CERTIFICATE OF CALIBRATION

Customer : EASTERN THAI CONSULTING 1992 CO., LTD.
683 Moo 11, Sukhapiban 8 Rd., Nongkham,
Sriracha, Chonburi 20230

Location of Calibration : Asia Medical and Agricultural Laboratory and Research Center Public Company Limited
(Calibration Laboratory)

Equipment : Standard Weight 50 g

Manufacturer : METTLER TOLEDO

Class : F1

Serial No. : N/A

ID No. : LABE 10/1

Date of Receipt : 18 May 2022

Date of Calibration : 30 May 2022

Calibrated by : Mr. Somwang Sangdee
Scientist
Approved by : (Mr. Somchai Neampunt)
Signed for Director

Issue date : 31 May 2022

The uncertainties are for a confidence probability of approximately 95%.

The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Asia Medical and Agricultural Laboratory and Research Center Public Company Limited (AMARC).



Certificate No. : 22-052238
Sample Code : 22-19150-003

REPORT OF CALIBRATION

Equipment : Standard Weight 50 g

Manufacturer : METTLER TOLEDO

Class : F1

Serial No. : N/A

ID No. : LABE 10/1

Result of Calibration :

☒ Without adjustment

☐ Adjustment

Conventional value of the result of weighing in air. For a weight taken at a reference temperature (t_{ref}) of 20°C, the conventional mass is the mass of a reference weight of a density (ρ_{ref}) of 8000 kg.m⁻³ which it balances in air of a reference density (ρ_0) of 1.2 kg.m⁻³

Description	Deviation	Conventional	Expanded	Maximum	ID No.
	(mg)	Mass	Uncertainty	Permissible Error	
			(mg)	\pm (mg)	
50 g	-0.324	49.999676 g	0.10	0.30	LABE 10/1

The result expanded uncertainty of measurement U is stated as the standard uncertainty multiplied by the coverage factor $k=2.0$, which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty of measurement has been determined in accordance with UKAS M3003

COPY

Certificate No. : 22-052238
Sample Code : 22-19150-003

REPORT OF CALIBRATION

Condition of Calibration

1. Ambient Conditions : Temperature $20^{\circ}\text{C} \pm 1.5^{\circ}\text{C}$, Relative humidity $50\% \pm 10\%$ and air density 1.20 kg/m^3
2. Calibration Method : Direct comparison weighing according to OIML R111-1 : 2004(E)
3. Reference standard instrument

Instrument	Class	ID No.	Certificate No.	Due Date
1) Standard Weight 1 mg to 1 kg	E2	LB-WE-79	21-078366	22 September 2022

4. This certification is traceable to the International System of Unit maintained at : -

Asia Medical and Agricultural Laboratory and Research Center Public Company Limited

(Instrument number 1).

5. Condition of Calibration item: Normal

6. Description of Calibrated Item :

Type and Nominal Value :	Standard Weight 50 g
Shape :	Cylindrical weight with knob
Material :	Stainless steel
Case :	Wooden Box
Comments :	Recalibration

- End of Report -

COPY



Certificate No. : 22-052239
Sample Code : 22-19150-004

Page 1 of 3

CERTIFICATE OF CALIBRATION

Customer : EASTERN THAI CONSULTING 1992 CO., LTD.
683 Moo 11, Sukhapiban 8 Rd., Nongkham,
Sriracha, Chonburi 20230

Location of Calibration : Asia Medical and Agricultural Laboratory and Research Center Public Company Limited
(Calibration Laboratory)

Equipment : Standard Weight 100 g

Manufacturer : N/A

Class : N/A

Serial No. : N/A

ID No. : LABE 10/2

Date of Receipt : 18 May 2022

Date of Calibration : 30 May 2022

Calibrated by : Mr. Somwang Sangdee
Scientist

(Mr. Somchai Neampunt)
Signed for Director

Issue date : 31 May 2022

The uncertainties are for a confidence probability of approximately 95%.

The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Asia Medical and Agricultural Laboratory and Research Center Public Company Limited (AMARC).



Certificate No. : 22-052239
Sample Code : 22-19150-004

REPORT OF CALIBRATION

Equipment : Standard Weight 100 g

Manufacturer : N/A

Class : N/A

Serial No. : N/A

ID No. : LABE 10/2

Result of Calibration : ☒ Without adjustment ☐ Adjustment

Conventional value of the result of weighing in air. For a weight taken at a reference temperature (t_{ref}) of 20°C, the conventional mass is the mass of a reference weight of a density (ρ_{ref}) of 8000 kg.m⁻³ which it balances in air of a reference density (ρ_a) of 1.2 kg.m⁻³

Description	Deviation (mg)	Conventional Mass	Expanded Uncertainty (mg)	Maximum Permissible Error \pm (mg)	ID No.
100 g	-0.171	99.999829 g	0.16	0.50	LABE 10/2

The result expanded uncertainty of measurement U is stated as the standard uncertainty multiplied by the coverage factor $k = 2.0$, which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty of measurement has been determined in accordance with UKAS M3003

COPY



Certificate No. : 22-052239

Sample Code : 22-19150-004

Page 3 of 3

REPORT OF CALIBRATION

Condition of Calibration

1. Ambient Conditions : Temperature 20 °C ± 1.5°C, Relative humidity 50% ± 10% and air density 1.18 kg/m³

2. Calibration Method : WI-CL-007 base on OIML R 111-1 : 2004(E)

3. Reference standard instrument

Instrument	Class	ID No.	Certificate No.	Due Date
1) Standard Weight 1 mg to 1 kg	E2	LB-WE-78	21-079366	22 September 2022

4. This certification is traceable to the International System of Unit maintained at :-

Asia Medical and Agricultural Laboratory and Research Center Public Company Limited

(Instrument number 1).

5. Condition of Calibration item: Normal

6. Description of Calibrated item :

Type and Nominal Value :	Standard Weight 100 g
Shape :	Cylindrical weight with knob
Material :	Stainless steel
Case :	Wooden Box
Comments :	Recalibration

- End of Report -

COPY



Certificate No. : 22-052237

Sample Code : 22-19150-002

CERTIFICATE OF CALIBRATION

Customer : EASTERN THAI CONSULTING 1992 CO., LTD.

689 Moo 11, Sukhapiban 8 Rd., Nongkham,

Siracha, Chonburi 20230

Location of Calibration : Asia Medical and Agricultural Laboratory and Research Center Public Company Limited
(Calibration Laboratory)

Equipment : Standard Weight 50 g

Manufacturer : N/A

Class : N/A

Serial No. : N/A

ID No. : LABE 10/4

Date of Receipt : 18 May 2022

Date of Calibration : 30 May 2022

Calibrated by : Mr. Somwang Sangdee
Scientist

Issue date : 31 May 2022

The uncertainties are for a confidence probability of approximately 95%.

The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Asia Medical and Agricultural Laboratory and Research Center Public Company Limited (AMARC).



Certificate No. : 22-052237

Sample Code : 22-19150-002

REPORT OF CALIBRATION

Equipment : Standard Weight 50 g

Manufacturer : N/A

Class : N/A

Serial No. : N/A

ID No. : LABE 10/4

Result of Calibration :

☒ Without adjustment☐ Adjustment

Conventional value of the result of weighing in air. For a weight taken at a reference temperature (t_{ref}) of 20°C, the conventional mass is the mass of a reference weight of a density (ρ_{ref}) of 8000 kg.m⁻³ which it balances in air of a reference density (ρ_0) of 1.2 kg.m⁻³

Description	Deviation	Conventional	Expanded	Maximum	ID No.
		Mass	Uncertainty	Permissible Error	
	(mg)		(mg)	± (mg)	
50 g	-0.111	49.999889 g	0.10	0.30	LABE 10/4

The result expanded uncertainty of measurement U is stated as the standard uncertainty multiplied by the coverage factor $k=2.0$, which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty of measurement has been determined in accordance with UKAS M3003

COPY



Certificate No. : 22-052237

Sample Code : 22-19150-002

Page 3 of 3

REPORT OF CALIBRATION

Condition of Calibration

1. Ambient Conditions : Temperature 20 °C ± 1.5°C, Relative humidity 50% ± 10% and air density 1.18 kg/m³
2. Calibration Method : WI-CL-007 base on OIML R 111-1 : 2004(E)

3. Reference standard instrument

Instrument	Class	ID No.	Certificate No.	Due Date
1) Standard Weight 1 mg to 1 kg	E2	LB-WE-79	21-079366	22 September 2022

4. This certification is traceable to the International System of Unit maintained at :-

Asia Medical and Agricultural Laboratory and Research Center Public Company Limited

(Instrument number 1).

5. Condition of Calibration item: Normal

6. Description of Calibrated Item :

Type and Nominal Value :	Standard Weight 50 g
Shape :	Cylindrical weight with knob
Material :	Stainless steel
Case :	Wooden Box
Comments :	Recalibration

- End of Report -

COPY