

ภาคผนวก จ

เอกสารสอบเทียบเครื่องมือ

การตรวจวัดคุณภาพสิ่งแวดล้อม
บริษัท พี.เอส.ซี สตาร์ช โปรดักส์ จำกัด (มหาชน)
ประจำปี 2567

List of Instruments Certification for Environmental Quality Analysis

No.	Instrument/Equipment	Parameter	Manufacturer	Model/Serial No.	Calibrator	Certification No.	Date of Calibration	Due date of Calibration*	Remark
Equipment for Air Quality Analysis									
1	Analytical Balance (Readability 0.1 mg)	ฝุ่นละอองรวม (TSP) ฝุ่นทุกขนาด (Total Dust)	Mettler-Toledo	MS204TS/00 C252436235	National Food Institute, Ministry of Industry, Thailand	2402420-003-01	19 Apr 24	18 Apr 25	-
2	Analytical Balance (Readability 0.001 mg)	Respirable Dust	Mettler-Toledo	XP6 / B322373893	National Food Institute, Ministry of Industry, Thailand	2402420-002-01	19 Apr 24	18 Apr 25	-
3	UV-VIS Spectrophotometer	ก๊าซไนโตรเจนไดออกไซด์ (NOx)	Agilent Technologies	Cary60 G6860A / MY15410009	DQE Services Co.,Ltd.	SP24-018	7 May 24	6 May 25	-
4	Ion Chromatography (IC)	ไฮโดรเจนคลอไรด์ (HCl), กรดซัลฟิวริก (H ₂ SO ₄), ไอโอดีน (I) คลอไรด์ (Cl), โซเดียมไฮโปคลอไรท์ ในรูปของคลอไรด์ (NaOCl as Cl) ไฮโดรเจนซัลไฟด์ (H ₂ S)	Dionex	DionexAqionRFC / 220380031	Archemica Lab Co.Ltd.	Qualification Report Anion (ID#1047)	23 Apr 24	22 Apr 25	-
5	Atomic Absorption Spectrophotometer (AAS)	เหล็ก (Fe), นิกเกิล (Ni), โครเมียม (Cr) อะลูมิเนียม (Al) แมกนีเซียมซัลเฟต ในรูปของแมกนีเซียม	Perkin Elmer	PinAAcle 900F / PFBS20031902	Perkin Elmer Co.,Ltd.	Preventive Maintenance Report	14 May 24	13 May 25	-
6	Inductively Coupled Plasma (ICP)	โซเดียมคาร์บอเนต ในรูปของโซเดียม แมงกานีส (Mn)	Agilent Technologies	System ID:G8015A G8015AA / MY18030001	Agilent Technologies (Thailand) Co.,Ltd.	Preventive Maintenance Checklist	4 Nov 24	3 Nov 25	-
Equipment for Water Quality Analysis									
7	pH Meter	ความเป็นกรด-ด่าง (pH) อุณหภูมิ (Temperature)	Mettler-Toledo	Seven Easy S20 / 1231155210	National Food Institute, Ministry of Industry, Thailand	2401718-001-01	11 Mar 24	10 Mar 25	-
8	pH Meter		Mettler-Toledo	Seven Easy S20 / 1230525212	DKSH (Thailand) Ltd.	C07240167	9 Apr 24	8 Apr 25	-
9	BOD Incubator	ความต้องการออกซิเจนทางชีวเคมี (BOD)	Arco	UC4-1320 / (UAE.WAO.015/2561)	Technology Promotion Association (Thailand-Japan)	24TM303	10 Feb 24	9 Feb 25	-
10	DO Meter		YSI	5100 / 11B101863	Technology Promotion Association (Thailand-Japan)	24TW39	21 Feb 24	20 Feb 25	-
11	Analytical Balance (Readability 0.1 mg)	น้ำมันและไขมัน (Fat Oil and Grease)	Mettler-Toledo	XSR204 / C117635043	Technology Promotion Association (Thailand-Japan)	24MM293	11 May 24	10 May 25	-

List of Instruments Certification for Environmental Quality Analysis

No.	Instrument/Equipment	Parameter	Manufacturer	Model/Serial No.	Calibrator	Certification No.	Date of Calibration	Due date of Calibration*	Remark
Equipment for Water Quality Analysis									
12	Analytical Balance (Readability 0.01 mg)	ของแข็งทั้งหมด (Total Solid) สารแขวนลอย (SS)	Mettler-Toledo	XSR205DU / C210685394	National Food Institute, Ministry of Industry, Thailand	2402283-002-01	2 Apr 24	1 Apr 25	-
13	Hot Air Oven	ปริมาณของแข็งแขวนลอยทั้งหมด (TSS) ปริมาณของแข็งละลายน้ำ (TDS)	Memmert	UF55 / B216.1666	National Food Institute, Ministry of Industry, Thailand	2500116-001-01	8 Oct 24	7 Oct 25	-
14	COD Reactor (Heating Block)	ความต้องการออกซิเจนทางเคมี (COD)	Hanna	HI839800 / 1147807	Hanna Instruments (Thailand) Ltd.	HIT-2417-0568	25 Apr 24	24 Apr 25	-
15	Digestor Unit	ทีเคเอ็น (TKN)	FOSS TECATOR	DT2520 / 91794469	National Food Institute, Ministry of Industry, Thailand	2402957-001-01	23 May 24	22 May 25	-
16	Distillation Unit (Kjeldahl Method)		FOSS TECATOR	KT200 / 91790524	FOSS South East Asia	9810	9 Feb 24	7 Feb 25	-
17	Atomic Absorption Spectrophotometer (AAS)	เหล็ก (Fe) นิกเกิล (Ni) โครเมียม (Cr)	Agilent Technologies	System ID:G8432A AA240FS / MY13160001	Thailand Institute of Scientific and Technological Research(TISTR)	MTC.ACL.No 358/67	11 Mar 24	10 Mar 25	-
18	Inductively Coupled Plasma (ICP)	ตะกั่ว (Pb)	Agilent Technologies	System ID:G8015A G8015AA / MY18030001	Agilent Technologies (Thailand) Co.,Ltd.	Preventive Maintenance Checklist	4 Nov 24	3 Nov 25	-

Calibration Certificate

Certificate No.: 2402420-003-01
Client name: UNITED ANALYST AND ENGINEERING CONSULTANT CO., LTD.
Address: 3 Soi Udomsuk 41, Sukhumvit Road,
Bangchack, Prakhonong, Bangkok 10260

Page 1 of 3

Equipment: Electronic Balance
Manufacturer: METTLER TOLEDO
Model: MS204TS/00
Serial No.: C252436235
ID No.: UAE.AIR.023/2566
Order No.: 2402420
Operation No.: 2402420-003
Date of Receipt: 19 April 2024
Date of Calibration: 19 April 2024

Calibrated by Mr.Pheraphat Tuanjit
Scientist
Approved by *P. Jaenghanit*
(Miss Preeyaporn Jaengkanit)
Vice President, Department of Laboratory Services
Responsible for the Technical Management Team
Date of Issue: 23 April 2024

The uncertainties are for a confidence probability of approximately 95%
This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the National Food Institute.

F-CS-009 Revision: 01 Date: 20-04-65

Calibration Report

Certificate No.: 2402420-003-01
Equipment: Electronic Balance
Model: MS204TS/00
Serial No.: C252436235
Capacity: 220 g
Manufacturer: METTLER TOLEDO
Resolution: 0.0001 g
ID No.: UAE.AIR.023/2566

Page 2 of 3

Date of Calibration: 19 April 2024

Environment Condition: Ambient Temperature: 21.7 ± 1.5 °C Relative Humidity: 65 ± 6.7 %

Place of Calibration: Room 206 Balance Room 2, UNITED ANALYST AND ENGINEERING CONSULTANT CO., LTD.

Condition of Equipment: Good Condition

Condition of This Results of Calibration:

1. Calibration Method: NF1 Method W-MA-001 In-House Method based on UKAS Lab 14 : 2019

2. Reference Standards:

Reference Standard	Model	Serial No.	Calibrated By	Certificate No.	Due Date
Standard Weight Class E2	1-500mg	15880	TCS	M23111815	28 November 2024
Standard Weight Class E2	1-500g	15882	TCS	M23111825	28 November 2024

Instrument	Model	Serial No.	Calibrated By	Certificate No.	Due Date
Thermo-Hygro Meter	608-H1	NFLBTH 019/23	Quality Reborn	QR24-0492	4 March 2025

3. This certification is traceable to SI UNIT

4. This certificate was certified only for the instrument we calibrated.

5. This result of calibration was found accurate as shown on date and place of calibration only.

Calibration Results:




1. Repeatability of Reading:

Nominal Value (g)	Standard Deviation of Reading (g)
100	0.000074
200	0.000074

2. Off-Center Error:

A mass of 100 g was placed and moved to various position on pan.

The balance reading obtained is given in the table.



1	2	3	4	5	6	(Maximum Difference)
(g)	(g)	(g)	(g)	(g)	(g)	(g)
100.0005	100.0006	100.0003	100.0006	100.0003	100.0005	0.0002

F-CS-012 Revision: 01 Date: 20-04-65

Calibration Report

Certificate No.: 2402420-003-01
Equipment: Electronic Balance
Model: MS204TS/00
Serial No.: C252436235
Capacity: 220 g
Manufacturer: METTLER TOLEDO
Resolution: 0.0001 g
ID No.: UAE.AIR.023/2566

Page 3 of 3

Date of Calibration: 19 April 2024

Calibration Results: (Continued)

Calibration Range: 0-200 g

Calibration Adjustment: Internal Calibration

3. Departure from Nominal Value:

Nominal Value (g)	Standard Value (g)	Average Reading (g)	Correction (g)	Uncertainty (g)	Coverage Factor k
Unload	0.00000	0.0000	0.0000	0.000094	2.00
0.1	0.10000	0.1000	0.0000	0.000094	2.00
1	0.99998	1.0000	0.0000	0.000097	2.00
5	4.99997	5.0000	0.0000	0.000096	2.00
10	10.00002	10.0000	0.0000	0.00012	2.00
20	20.00003	20.0001	-0.0001	0.00014	2.00
50	49.99998	50.0003	-0.0003	0.00012	2.00
70	70.00000	70.0005	-0.0005	0.00017	2.00
100	99.99997	100.0006	-0.0006	0.00017	2.00
150	149.99994	150.0012	-0.0013	0.00022	2.00
200	200.00001	200.0015	-0.0015	0.00028	2.00

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k, providing a level of confidence of approximately 95 %.

----- End -----

F-CS-012 Revision: 01 Date: 20-04-65

Calibration Certificate

Certificate No.: 2402420-002-01
Client name: UNITED ANALYST AND ENGINEERING CONSULTANT CO., LTD.
Address: 3 Soi Udomsuk 41, Sukhumvit Road,
Bangchack, Prakhonong, Bangkok 10260

Page 1 of 3

Equipment: Electronic Balance
Manufacturer: METTLER TOLEDO
Model: XP6
Serial No.: B322373893
ID No.: UAE.AIR.019/2556
Order No.: 2402420
Operation No.: 2402420-002
Date of Receipt: 19 April 2024
Date of Calibration: 19 April 2024

Calibrated by Mr.Pheraphat Tuanjit
Scientist
Approved by *P. Jaenghanit*
(Miss Preeyaporn Jaengkanit)
Vice President, Department of Laboratory Services
Responsible for the Technical Management Team
Date of Issue: 23 April 2024

The uncertainties are for a confidence probability of approximately 95%

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the National Food Institute.

F-CS-009 Revision: 01 Date: 20-04-65

Calibration Report

Certificate No.: 2402420-002-01

Equipment:

Electronic Balance

Model: XP6

Serial No.: 8322373893

Capacity: 6.1 g

Manufacturer: METTLER TOLEDO

Resolution: 0.000001 g

ID No.: UAE-AIR.019/2556

Date of Calibration: 19 April 2024

Page 2 of 3

Environment Condition: Ambient Temperature: 22.6 ± 1.8 °C Relative Humidity: 48 ± 6.0 %

Place of Calibration: Room 206 Balance Room 2, UNITED ANALYST AND ENGINEERING CONSULTANT CO., LTD.

Condition of Equipment: Good Condition

Condition of This Results of Calibration:

1. Calibration Method: NFI Method W-MA-001 In-House Method based on UKAS Lab 14 : 2019

2. Reference Standards:

Reference Standard	Model	Serial No.	Calibrated By	Certificate No.	Due Date
Standard Weight Class E2	1-500mg	15880	TCS	M23111815	28 November 2024
Standard Weight Class E2	1-500g	15882	TCS	M23111825	28 November 2024

Instrument	Model	Serial No.	Calibrated By	Certificate No.	Due Date
Thermo-Hygro Meter	608-H1	NFI.BTH 019/23	Quality Reborn	QR24-0492	4 March 2025

3. This certification is traceable to SI UNIT

4. This certificate was certified only for the instrument we calibrated.

5. This result of calibration was found accurate as shown on date and place of calibration only.

Calibration Results:


1. Repeatability of Reading:

Nominal Value (g)	Standard Deviation of Reading (g)
3	0.0000057
6	0.0000019

2. Off-Center Error:

A mass of 2 g was placed and moved to various position on pan.

The balance reading obtained is given in the table.



1	2	3	4	5	6	(Maximum Difference)
(g)	(g)	(g)	(g)	(g)	(g)	(g)
1.999981	1.999983	1.999980	1.999984	1.999983	1.999981	0.000003

F-CS-012 Revision: 01 Date: 20-04-65

2008 ถนนสุขุมวิท 35 นุสราภิรมย์ กรุงเทพมหานคร 10700
2008 Soi 35, Nua Amarin Road, Bang Yi Khan Subdistrict, Bang Phai District, Bangkok 10700, Thailand
Tel: +66(0) 2142 8668 Fax: +66(0) 2142 8645



nfi.or.th

Calibration Report

Certificate No.: 2402420-002-01

Equipment:

Electronic Balance

Model: XP6

Serial No.: 8322373893

Capacity: 6.1 g

Manufacturer: METTLER TOLEDO

Resolution: 0.000001 g

ID No.: UAE-AIR.019/2556

Date of Calibration: 19 April 2024

Page 3 of 3

Calibration Results: (Continued)

Calibration Range: 0-6 g

Calibration Adjustment: Internal Calibration

3. Departure from Nominal Value:

Nominal Value (g)	Standard Value (g)	Average Reading (g)	Correction (g)	Uncertainty (± g)	Coverage Factor k
Unit	0.0000000	0.000000	0.000000	0.0000032	2.00
0.01	0.0099970	0.009999	-0.000002	0.0000047	2.00
0.05	0.0500010	0.050003	-0.000002	0.0000048	2.00
0.10	0.1000010	0.100001	0.000000	0.0000069	2.00
0.15	0.1500020	0.150002	0.000000	0.0000083	2.00
0.17	0.1700050	0.170006	-0.000001	0.000012	2.00
0.20	0.1999990	0.200002	-0.000003	0.0000083	2.00
1.50	1.4999750	1.499971	0.000004	0.000027	2.00
3.00	2.9999680	2.999959	0.000009	0.000028	2.00
4.50	4.4999810	4.499967	0.000014	0.000022	2.00
6.00	5.9999490	5.999931	0.000018	0.000032	2.00

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k, providing a level of confidence of approximately 95 %.

***** End *****

F-CS-012 Revision: 01 Date: 20-04-65

2008 ถนนสุขุมวิท 35 นุสราภิรมย์ กรุงเทพมหานคร 10700
2008 Soi 35, Nua Amarin Road, Bang Yi Khan Subdistrict, Bang Phai District, Bangkok 10700, Thailand
Tel: +66(0) 2142 8668 Fax: +66(0) 2142 8645



nfi.or.th

DQE Services Co.,Ltd.

32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Bangkok 10230

Phone : +66 (0)2 538 2054, Email : dqeservicesinfo@gmail.com



CERTIFICATE OF CALIBRATION

Certificate No. : SP24-018

Page 1 of 5

Customer : United Analyst and Engineering Consultant Co.,Ltd. (Head Office)

Address : 3 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260

Location of calibration : Laboratory 315

Equipment : UV-Vis Spectrophotometer

Manufacturer : Agilent Technologies

Model : Cary 60

Serial No. : MY15410009

ID No. : UAE.WAT.020/2558

Received Date : 7 May 2024

Calibration Date : 7 May 2024

Issue Date : 9 May 2024

Condition Instrument : Good

Calibrated by : 
(Mr. Tanawat Rittidach)

Approved by : 
(Ms. Chonthicha Sangnorn)

Technical Manager

Quality Manager

The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only.

The measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the DQE Services Co., Ltd.

DQE Services Co.,Ltd.

32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Bangkok 10230

Phone : +66 (0)2 538 2054, Email : dqeservicesinfo@gmail.com



REPORT OF CALIBRATION

Certificate No. : SP24-018

Page 2 of 5

Environment Condition : Ambient Temperature 25 ± 5 °C

Relative humidity 55 ± 20 %RH

Calibration method : In-house method CP-01 Based on ASTM E275-08

Certified Reference Materials :

Material	Serial No.	Certificate No.	Due date
Absorbance Standard set	25760	115663	25 October 2025
Absorbance Standard set	25757	115638	25 October 2025
Wavelength Standard set	25806	115657	25 October 2025
Wavelength Standard set	25758	115665	25 October 2025

Traceability : This certification is traceable to the International System of Unit maintained at National -

Institute of Standards and Technology (NIST) through Starna Scientific Limited

Spectral Band Width of UUC : 1.5 nm.

Scan Speed of UUC : 60 nm/min

Scan Interval of UUC : 0.15 nm.

Resolution of UUC : Photometric 0.0001 Abs.

Wavelength 0.1 nm.

เอกสารไม่ควบคุม

เอกสารไม่ควบคุม

REPORT OF CALIBRATION

Certificate No. : SP24-018

Page 3 of 5

Calibration Results : Without adjustment

Photometric Accuracy :

Wavelength (nm.)	CRMs Values (Abs)	UUC Reading (Abs)	Correction (Abs)	Uncertainty (Abs)	Coverage factor k
420	0.0000	0.0000	0.0000	0.0028	2.00
	0.5780	0.5747	0.0033	0.0031	2.00
	1.0484	1.0438	0.0046	0.0029	2.00
	2.1876	2.1832	0.0044	0.0080	2.00
440	0.0000	0.0000	0.0000	0.0028	2.00
	0.5595	0.5581	0.0014	0.0034	2.00
	1.0239	1.0231	0.0008	0.0035	2.00
	2.1230	2.1219	0.0011	0.0080	2.00
465	0.0000	0.0000	0.0000	0.0028	2.00
	0.5230	0.5184	0.0046	0.0030	2.00
	0.9633	0.9614	0.0019	0.0029	2.00
	1.9753	1.9731	0.0022	0.0070	2.00
546.1	0.0000	0.0000	0.0000	0.0028	2.00
	0.5181	0.5150	0.0031	0.0031	2.00
	1.0002	0.9964	0.0038	0.0033	2.00
	1.9973	1.9914	0.0059	0.0088	2.00
590	0.0000	0.0000	0.0000	0.0028	2.00
	0.5517	0.5485	0.0032	0.0030	2.00
	1.0803	1.0772	0.0031	0.0030	2.00
	2.0373	2.0293	0.0080	0.0080	2.00
635	0.0000	0.0000	0.0000	0.0028	2.00
	0.5591	0.5565	0.0026	0.0031	2.00
	1.0518	1.0482	0.0036	0.0030	2.00
	1.9274	1.9202	0.0072	0.0079	2.00

เอกสารไม่ควบคุม

REPORT OF CALIBRATION

Certificate No. : SP24-018

Page 4 of 5


Photometric Accuracy :

Wavelength (nm.)	CRMs Values (Abs)	UUC Reading (Abs)	Correction (Abs)	Uncertainty (Abs)	Coverage factor k
235	0.0000	0.0000	0.0000	0.0050	2.00
	0.7469	0.7435	0.0034	0.0057	2.00
257	0.0000	0.0000	0.0000	0.0050	2.00
	0.8674	0.8639	0.0035	0.0060	2.00
313	0.0000	0.0000	0.0000	0.0050	2.00
	0.2919	0.2907	0.0012	0.0051	2.00
350	0.0000	0.0000	0.0000	0.0050	2.00
	0.6430	0.6402	0.0028	0.0055	2.00

เอกสารไม่ควบคุม

DQE Services

DQE Services Co.,Ltd.
32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Bangkok 10230
Phone : +66 (0)2 538 2054, Email : dqeservicesinfo@gmail.com


ISO 15189:2013
CALIBRATION DATA

REPORT OF CALIBRATION					
Certificate No. : SP24-018			Page 5 of 5		
Wavelength Accuracy :					
CRMs Values (nm.)	UUC Reading (nm.)	Correction (nm.)	Uncertainty (nm.)	Coverage factor k	
241.72	242.0	-0.28	0.18	2.00	
279.45	279.5	-0.05	0.18	2.00	
287.81	287.9	-0.09	0.18	2.00	
334.06	333.9	0.16	0.18	2.00	
360.93	360.5	0.43	0.18	2.00	
418.59	418.1	0.49	0.18	2.00	
445.94	445.6	0.34	0.18	2.00	
453.66	453.3	0.36	0.18	2.00	
460.02	459.8	0.22	0.18	2.00	
536.59	536.0	0.59	0.18	2.00	
637.98	638.7	-0.72	0.18	2.00	
431.38	430.8	0.58	0.18	2.00	
472.50	472.4	0.10	0.18	2.00	
513.47	513.7	-0.23	0.18	2.00	
528.88	529.1	-0.22	0.18	2.00	
573.17	573.5	-0.33	0.18	2.00	
585.35	585.2	0.15	0.20	2.00	
684.40	685.1	-0.70	0.18	2.00	
740.72	741.4	-0.68	0.20	2.00	
748.55	749.1	-0.55	0.18	2.00	
807.03	807.3	-0.27	0.18	2.00	
879.28	879.3	-0.02	0.18	2.00	

Remark : - UUC = Unit Under Calibration
- N/A = Not Available
- The result expanded uncertainty of measurement U is stated as the standard uncertainty of measurement multiplied by the coverage factor k, which for a normal distribution corresponds to a coverage probability of approximately 95%
- * Indicates non TISI accredited

- End of Certificate -

เอกสารไม่ควบคุม


ARCHEMICA

Certificate of Calibration
AquionRFIC : Anion (ID#1047)
This certificate is to verify that instrument below are calibrated
by Archemica Lab Co.,Ltd.
AquionRFIC S/N : 220380031
AS-DV S/N : 220360045
for
United Analyst and Engineering Consultant Co.,Ltd.
Operator Signature : K. Channarong Date : Apr 23, 2024
(Mr.Channarong Khiao-Un)
Test Engineer

เอกสารไม่ควบคุม

Qualification Report

PM Check list, CM_OQ and PQ

AquionRFIC : Anion (ID#1047)

Aquion : Cation (ID#1048)

For

United Analyst Engineering Consultant Co.,Ltd.
(Validate System 2024)

PM Anion ID#1047

Preventive Maintenance Check List

เอกสารไม่ควบคุม

เอกสารไม่ควบคุม



Checklist ICS Preventive Maintenance

Dionex Ion Chromatography Preventive Maintenance Report

Customer Organization	Name/ Department
United Analyst and Engineering Consultant Co.,Ltd.	Khun.Suwan Kongthong / Lab
Engineer	Date
Mr.Channarong Khiao-Un	23-24/Apr/2024

Instrument Detail

Instrument Model	Application
AquionRFIC	Anion
Instrument components	Serial Number
AquionRFIC	220380031
AS-DV	220360045

Consumable Detail

Columns	Guard Columns	Suppressors	Concentrators	Etc.
AS18	AG18	ADRS-600	-	EGC III KOH
				CR-ATC

Remark: หมายเหตุ Column, Guard Column และ Suppressor มี peak shift และ tail

Perform By Archemica

K. Channarong
Archemica
23/Apr/2024

Suron
Customer
23/Apr/2024

เอกสารไม่ควบคุม



Checklist ICS Preventive Maintenance

General ICS Maintenance Checklist

No.	Description	Result			
		Checked	Cleaned	Replaced	N.A.
Power on & Connection					
1	Instrument power on	<input checked="" type="checkbox"/>	-	-	<input type="checkbox"/>
2	Instrument connection	<input checked="" type="checkbox"/>	-	-	<input type="checkbox"/>
Injection Valve Rebuild		Checked	Cleaned	Replaced	N.A.
3	Rebuilt injection valve 6 port	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
4	- Rotor seal	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
5	- Stator face	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
(Optional) Auxiliary Valve Rebuild		Checked	Cleaned	Replaced	N.A.
6	Rebuilt auxiliary valve - port	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>
7	- Rotor seal	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>
8	- Stator face	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>
Check Valve Cartridge		Checked	Cleaned	Replaced	N.A.
9	Inlet check valve assembly	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
10	Outlet check valve assembly	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
11	Verified correct flow orientation	<input checked="" type="checkbox"/>	-	-	<input type="checkbox"/>
Pump Piston Rinse Seal, Piston Seal and Piston		Checked	Cleaned	Replaced	N.A.
12	Piston rinse seal in primary pump head	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
13	Piston seal in primary pump head	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
14	Piston in primary pump head	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
15	Piston rinse seal in secondary pump head	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
16	Piston seal in secondary pump head	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
17	Piston in secondary pump head	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Waste Valve and Priming Valve		Checked	Cleaned	Replaced	N.A.
18	Waste valve	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
19	Priming valve	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Cell Detector		Checked	Cleaned	Replaced	N.A.
20	Check conductivity cell	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
21	Check electrochemical cell	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>
22	- Working electrode	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>
23	- Reference electrode	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>
24	- Gasket	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>
25	- Cell body	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>
Other		Checked	Cleaned	Replaced	N.A.
26	Sample Loop Size 25 uL	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
27	End-line filter	<input checked="" type="checkbox"/>	-	<input type="checkbox"/>	<input type="checkbox"/>
28	Leak sensor	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
29	Lubricate pump mechanic	<input type="checkbox"/>	Lubricated	-	<input type="checkbox"/>
30	Reconnected liquid lines to the valve	<input checked="" type="checkbox"/>	-	-	<input type="checkbox"/>
31	Reconnected liquid lines to pump heads	<input checked="" type="checkbox"/>	-	-	<input type="checkbox"/>
32	Primed pump	<input checked="" type="checkbox"/>	-	-	<input type="checkbox"/>
33	Checked pump for leaks	<input checked="" type="checkbox"/>	-	-	<input type="checkbox"/>
34	Checked gas for leaks	<input checked="" type="checkbox"/>	-	-	<input type="checkbox"/>

เอกสารไม่ควบคุม



AS-DV Autosampler Preventive Maintenance Checklist

Model	Serial number	Firmware Version
<input checked="" type="checkbox"/> AS-DV	220360045	1.6.0

No.	Description	Result			
Power on & Connection		Checked	Cleaned	Replaced	N.A.
1.	AS-DV power on	<input checked="" type="checkbox"/>	-	-	<input type="checkbox"/>
2.	AS-DV connection	<input checked="" type="checkbox"/>	-	-	<input type="checkbox"/>
Sampling Tip		Checked	Cleaned	Replaced	N.A.
3.	Sampling needle	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
4.	Sampling tubing (Transfer line)	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
5.	Reconnect sampling needle & tubing	<input checked="" type="checkbox"/>	-	-	<input type="checkbox"/>
Other		Checked	Cleaned	Replaced	N.A.
6.	Check carousel movement	<input checked="" type="checkbox"/>	-	-	<input type="checkbox"/>
7.	Check needle movement	<input checked="" type="checkbox"/>	-	-	<input type="checkbox"/>
8.	Lubricate needle drive	<input type="checkbox"/>	<input checked="" type="checkbox"/> Lubricated	-	<input type="checkbox"/>
9.	AS-DV cover	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
(Optional) High Pressure Valve		Checked	Cleaned	Replaced	N.A.
10.	High pressure valve - Port	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>
11.	- Rotor seal	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>
12.	- Stator face	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>
13.	- Reconnected liquid line to the valve	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>

Others / comments

เอกสารไม่ควบคุม

Dionex Ion Chromatography
Preventive Maintenance Report

Customer Organization	Name/ Department
United Analyst and Engineering Consultant Co.,Ltd.	Khun.Suwan Kongthong / Lab
Engineer	Date
Mr.Channarong Khiao-Un	23-24/Apr/2024

Instrument Detail

Instrument Model	Application
Aquion	Cation
Instrument components	Serial Number
Aquion	220340349

Consumable Detail

Columns	Guard Columns	Suppressors	Concentrators	Etc.
CS12A	CG12A	CDER-600	-	-
Remark: ขณะนี้ไม่มีเครื่องให้ร่นถ่าย, System ยังไม่มีการ				

Perform By Archemica

Archemica

Date

23/Apr/2024



Customer

Date

เอกสารไม่ควบคุม

PM Cation ID#1048

Preventive Maintenance
Check List

General ICS Maintenance Checklist

No.	Description	Result			
Power on & Connection		Checked	Cleaned	Replaced	N.A.
1	Instrument power on	<input checked="" type="checkbox"/>	-	-	<input type="checkbox"/>
2	Instrument connection	<input checked="" type="checkbox"/>	-	-	<input type="checkbox"/>
Injection Valve Rebuild		Checked	Cleaned	Replaced	N.A.
3	Rebuilt injection valve & port	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
4	- Rotor seal	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
5	- Stator face	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
(Optional) Auxiliary Valve Rebuild		Checked	Cleaned	Replaced	N.A.
6	Rebuilt auxiliary valve - port	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>
7	- Rotor seal	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>
8	- Stator face	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>
Check Valve Cartridge		Checked	Cleaned	Replaced	N.A.
9	Inlet check valve assembly	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
10	Outlet check valve assembly	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
11	Verified correct flow orientation	<input checked="" type="checkbox"/>	-	-	<input type="checkbox"/>
Pump Piston Rinse Seal, Piston Seal and Piston		Checked	Cleaned	Replaced	N.A.
12	Piston rinse seal in primary pump head	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
13	Piston seal in primary pump head	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
14	Piston in primary pump head	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
15	Piston rinse seal in secondary pump head	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
16	Piston seal in secondary pump head	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
17	Piston in secondary pump head	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Waste Valve and Priming Valve		Checked	Cleaned	Replaced	N.A.
18	Waste valve	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
19	Priming valve	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Cell Detector		Checked	Cleaned	Replaced	N.A.
20	Check conductivity cell	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
21	Check electrochemical cell	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>
22	- Working electrode	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>
23	- Reference electrode	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>
24	- Gasket	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>
25	- Cell body	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>
Other		Checked	Cleaned	Replaced	N.A.
26	Sample Loop Size 25 uL	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
27	End-line filter	<input type="checkbox"/>	-	<input type="checkbox"/>	<input type="checkbox"/>
28	Leak sensor	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
29	Lubricate pump mechanic	<input type="checkbox"/>	<input checked="" type="checkbox"/> Lubricated	-	<input type="checkbox"/>
30	Reconnected liquid lines to the valve	<input checked="" type="checkbox"/>	-	-	<input type="checkbox"/>
31	Reconnected liquid lines to pump heads	<input checked="" type="checkbox"/>	-	-	<input type="checkbox"/>
32	Primed pump	<input checked="" type="checkbox"/>	-	-	<input type="checkbox"/>
33	Checked pump for leaks	<input checked="" type="checkbox"/>	-	-	<input type="checkbox"/>
34	Checked gas for leaks	<input checked="" type="checkbox"/>	-	-	<input type="checkbox"/>

เอกสารไม่ควบคุม

CM OQ

Chromeleon Operation Qualification

ThermoFisher SCIENTIFIC Chromeleon Operational Qualification

General Information

Computer Name Version Number:
Instrument Controller: DESKTOP-C4FS3L7 7.3.1 Build 6535
Client: DESKTOP-C4FS3L7 7.3.1.6535
Operator: Mr.Channarong Khiao-Un
Overall Test Result: **Passed**

Comparison Format:

All Parameters:	Significant Digits:	10
-----------------	---------------------	----



K.Channarong 23/Apr/2024

Reviewer's Signature // Date

Operator's Signature // Date

เอกสารไม่ควบคุม

เอกสารไม่ควบคุม

ThermoFisher SCIENTIFIC Chromeleon Operational Qualification, Part 1 Verification of Selected Results

Detection Algorithm: Cobra
Calibration Type: Lin, WithOffset
Evaluation Type: Area
Standard Method: External
Calibration Mode: Total

Report Variable	Peak Name	Status
Offset (c0)	Acetanilide	ok
	Acetophenone	ok
	Propiophenone	ok
Slope (c1)	Acetanilide	ok
	Acetophenone	ok
	Propiophenone	ok
Correlation Coeff.	Acetanilide	ok
	Acetophenone	ok
	Propiophenone	ok
Variance	Acetanilide	ok
	Acetophenone	ok
	Propiophenone	ok
Std. Deviation	Acetanilide	ok
	Acetophenone	ok
	Propiophenone	ok
Rel. Std. Dev.	Acetanilide	ok
	Acetophenone	ok
	Propiophenone	ok
Variance Coeff.	Acetanilide	ok
	Acetophenone	ok
	Propiophenone	ok

ThermoFisher SCIENTIFIC Chromeleon Operational Qualification, Part 1 Verification of Selected Results

Report Variable	Peak Name	Status
Calibration Point X	Acetanilide	ok
	Acetophenone	ok
	Propiophenone	ok
Calibration Point Y	Acetanilide	ok
	Acetophenone	ok
	Propiophenone	ok
Amount [ng]	Acetanilide	ok
	Acetophenone	ok
	Propiophenone	ok
Resolution (EP)	Acetanilide	ok
	Acetophenone	ok
Resolution (USP)	Acetanilide	ok
	Acetophenone	ok
Peak Asymmetry (EP/USP)	Acetanilide	ok
	Acetophenone	ok
	Propiophenone	ok
Peak Asymmetry (AIA)	Acetanilide	ok
	Acetophenone	ok
	Propiophenone	ok

เอกสารไม่ควบคุม

เอกสารไม่ควบคุม



Chromeleon Operational Qualification, Part 1
Verification of Selected Results

Report Variable	Peak Name	Status
Theoretical Plates (EP)	Acetanilide	ok
	Acetophenone	ok
	Propiophenone	ok
Theoretical Plates (USP)	Acetanilide	ok
	Acetophenone	ok
	Propiophenone	ok
Theoretical Plates (JP)	Acetanilide	ok
	Acetophenone	ok
	Propiophenone	ok

Test Result: Passed



Chromeleon Operational Qualification, Part 2
Most Frequently Used Parameters: Comparison with Expected Results

Detection Algorithm: Cobra
Calibration Type: Lin, WithOffset
Evaluation Type: Area
Standard Method: External
Calibration Mode: Total

Variable Category	Report Variable	Peak Name	Status
Injection	No.		ok
	Name		ok
	Type		ok
	Position		ok
	Status		ok
	Volume		ok
	Dilution Factor		ok
	Weight		ok
	IntStd		ok
	InstrumentMethod		ok
	ProcessingMethod		ok
Chromatogram	Channel		ok
	No. of Peaks		ok
	Chromatogram Start Time		ok
	Signal Min.		ok
	Signal Max.		ok
	Unit		ok
	Noise		ok
Peak Results	No.	Acetanilide	ok
	No.	Acetophenone	ok
	No.	Propiophenone	ok
	Peak Name	Acetanilide	ok
	Peak Name	Acetophenone	ok
	Peak Name	Propiophenone	ok
	Ret.Time	Acetanilide	ok
	Ret.Time	Acetophenone	ok
	Ret.Time	Propiophenone	ok
	Ret.Time	Propiophenone	ok

เอกสารไม่ควบคุม

เอกสารไม่ควบคุม



Chromeleon Operational Qualification, Part 2
Most Frequently Used Parameters: Comparison with Expected Results

Variable Category	Report Variable	Peak Name	Status
Peak Results	Abs.Ret.Dev.	Acetanilide	ok
	Ret.Dev.(abs)	Acetophenone	ok
	Ret.Dev.(abs)	Propiophenone	ok
	Ret.Ret.Dev.	Acetanilide	ok
	Ret.Dev.(rel)	Acetophenone	ok
	Ret.Dev.(rel)	Propiophenone	ok
	Area	Acetanilide	ok
	Area	Acetophenone	ok
	Area	Propiophenone	ok
	Rel.Area	Acetanilide	ok
	Rel.Area (Total)	Acetophenone	ok
	Rel.Area (Total)	Propiophenone	ok
	Height	Acetanilide	ok
	Height	Acetophenone	ok
	Height	Propiophenone	ok
	Rel.Height (Total)	Acetanilide	ok
	Rel.Height (Total)	Acetophenone	ok
	Rel.Height (Total)	Propiophenone	ok
	Amount	Acetanilide	ok
	Amount	Acetophenone	ok
	Amount	Propiophenone	ok
	Concentration	Acetanilide	ok
	Concentration	Acetophenone	ok
	Concentration	Propiophenone	ok
	Rel.Amount	Acetanilide	ok
	Rel.Amount	Acetophenone	ok
	Rel.Amount	Propiophenone	ok
	Peak Width (0%)	Acetanilide	ok
	Peak Width (0%)	Acetophenone	ok
	Peak Width (0%)	Propiophenone	ok
	Peak Width (5%)	Acetanilide	ok
	Peak Width (5%)	Acetophenone	ok
	Peak Width (5%)	Propiophenone	ok
	Peak Width (10%)	Acetanilide	ok
	Peak Width (10%)	Acetophenone	ok
	Peak Width (10%)	Propiophenone	ok

เอกสารไม่ควบคุม



Chromeleon Operational Qualification, Part 2
Most Frequently Used Parameters: Comparison with Expected Results

Variable Category	Report Variable	Peak Name	Status
Peak Results	Peak Width (50%)	Acetanilide	ok
	Peak Width (50%)	Acetophenone	ok
	Peak Width (50%)	Propiophenone	ok
	Left Width (0%)	Acetanilide	ok
	Left Width (0%)	Acetophenone	ok
	Left Width (0%)	Propiophenone	ok
	Right Width (0%)	Acetanilide	ok
	Right Width (0%)	Acetophenone	ok
	Right Width (0%)	Propiophenone	ok
	Peak Start	Acetanilide	ok
	Peak Start	Acetophenone	ok
	Peak Start	Propiophenone	ok
	Peak Stop	Acetanilide	ok
	Peak Stop	Acetophenone	ok
	Peak Stop	Propiophenone	ok
	Peak Start Value	Acetanilide	ok
	Peak Start Value	Acetophenone	ok
	Peak Start Value	Propiophenone	ok
	Peak Stop Value	Acetanilide	ok
	Peak Stop Value	Acetophenone	ok
	Peak Stop Value	Propiophenone	ok
	BL-Value Peak Start	Acetanilide	ok
	BL-Value Peak Start	Acetophenone	ok
	BL-Value Peak Start	Propiophenone	ok
	BL-Value Peak Stop	Acetanilide	ok
	BL-Value Peak Stop	Acetophenone	ok
	BL-Value Peak Stop	Propiophenone	ok
	Type	Acetanilide	ok
	Type	Acetophenone	ok
	Type	Propiophenone	ok
	Resolution (EP)	Acetanilide	ok
	Resolution (EP)	Acetophenone	ok
	Resolution (USP)	Acetanilide	ok
	Resolution (USP)	Acetophenone	ok
	Asymmetry (EP)	Acetanilide	ok
	Asymmetry (EP)	Acetophenone	ok
	Asymmetry (EP)	Propiophenone	ok

เอกสารไม่ควบคุม



Chromeleon Operational Qualification, Part 2

Most Frequently Used Parameters: Comparison with Expected Results

Variable Category	Report Variable	Peak Name	Status
Peak Results	Asymmetry(AIA)	Acetanilide	ok
	Asymmetry(AIA)	Acetophenone	ok
	Asymmetry(AIA)	Propiophenone	ok
	Theor. Plates(EP)	Acetanilide	ok
	Theor. Plates(EP)	Acetophenone	ok
	Theor. Plates(EP)	Propiophenone	ok
	Theor. Plates(USP)	Acetanilide	ok
	Theor. Plates(USP)	Acetophenone	ok
	Theor. Plates(USP)	Propiophenone	ok
	Theor.Plates (JP)	Acetanilide	ok
	Theor. Plates(JP)	Acetophenone	ok
	Theor. Plates(JP)	Propiophenone	ok
Peak Calibration	Cal.Mode	Acetanilide	ok
	Cal.Mode	Acetophenone	ok
	Cal.Mode	Propiophenone	ok
	Cal.Type	Acetanilide	ok
	Cal.Type	Acetophenone	ok
	Cal.Type	Propiophenone	ok
	Weights	Acetanilide	ok
	Weights	Acetophenone	ok
	Weights	Propiophenone	ok
	Calibr. Coefficient C0	Acetanilide	ok
	Calibr. Coefficient C0	Acetophenone	ok
	Calibr. Coefficient C0	Propiophenone	ok
	Calibr. Coefficient C1	Acetanilide	ok
	Calibr. Coefficient C1	Acetophenone	ok
	Calibr. Coefficient C1	Propiophenone	ok
	RF-Value	Acetanilide	ok
	RF-Value	Acetophenone	ok
	RF-Value	Propiophenone	ok
	No. of Points	Acetanilide	ok
	No. of Points	Acetophenone	ok

เอกสารไม่ควบคุม



Chromeleon Operational Qualification, Part 2

Most Frequently Used Parameters: Comparison with Expected Results

Variable Category	Report Variable	Peak Name	Status
Peak Calibration	Residual for Cal.Point X	Acetanilide	ok
	Residual for Cal.Point X	Acetophenone	ok
	Residual for Cal.Point X	Propiophenone	ok
	Calibration Point Status	Acetanilide	ok
	Calibration Point Status	Acetophenone	ok
	Calibration Point Status	Propiophenone	ok
	Amount	Acetanilide	ok
	Amount	Acetophenone	ok
	Amount	Propiophenone	ok
Component	Cal.Type	Acetanilide	ok
	Peak Type	Acetanilide	ok
	Left Limit	Acetophenone	ok
	Right Limit	Acetanilide	ok
	Group	Acetanilide	ok
	Factor	Acetophenone	ok
	Amount	Acetanilide	ok
	Conc.Unit	Acetophenone	ok

เอกสารไม่ควบคุม



Chromeleon Operational Qualification, Part 2

Most Frequently Used Parameters: Comparison with Expected Results

Variable Category	Report Variable	Peak Name	Status
Peak Calibration	No. of Points	Propiophenone	ok
	No. of Points(disabled)	Acetanilide	ok
	No. of Points(disabled)	Acetophenone	ok
	No. of Points(disabled)	Propiophenone	ok
	Variance	Acetanilide	ok
	Variance	Acetophenone	ok
	Variance	Propiophenone	ok
	Var.Coeff	Acetanilide	ok
	Var.Coeff	Acetophenone	ok
	Var.Coeff	Propiophenone	ok
	Std.Dev.	Acetanilide	ok
	Std.Dev.	Acetophenone	ok
	Std.Dev.	Propiophenone	ok
	Rel.Std.Dev.	Acetanilide	ok
	Rel.Std.Dev.	Acetophenone	ok
	Rel.Std.Dev.	Propiophenone	ok
	Corr.Coeff.	Acetanilide	ok
	Corr.Coeff.	Acetophenone	ok
	Corr.Coeff.	Propiophenone	ok
	R-Square	Acetanilide	ok
	R-Square	Acetophenone	ok
	R-Square	Propiophenone	ok
	Adj. R-Square	Acetanilide	ok
	Adj. R-Square	Acetophenone	ok
	Adj. R-Square	Propiophenone	ok
	X	Acetanilide	ok
	X	Acetophenone	ok
	X	Propiophenone	ok
	Y	Acetanilide	ok
	Y	Acetophenone	ok
	Y	Propiophenone	ok
	W	Acetanilide	ok
	W	Acetophenone	ok
	W	Propiophenone	ok
	F(X)	Acetanilide	ok
	F(X)	Acetophenone	ok
	F(X)	Propiophenone	ok

เอกสารไม่ควบคุม



Chromeleon Operational Qualification, Part 2

Most Frequently Used Parameters: Comparison with Expected Results

Variable Category	Report Variable	Peak Name	Status
Peak Purity	PPI	Acetanilide	ok
	PPI	Acetophenone	ok
	PPI	Propiophenone	ok
	RSD PPI	Acetanilide	ok
	RSD PPI	Acetophenone	ok
	RSD PPI	Propiophenone	ok
	Match	Acetanilide	ok
	Match	Acetophenone	ok
	Match	Propiophenone	ok
	RSD Match	Acetanilide	ok
	RSD Match	Acetophenone	ok
	RSD Match	Propiophenone	ok
	Rel.Max at	Acetanilide	ok
	Rel.Max at	Acetophenone	ok
	Rel.Max at	Propiophenone	ok

Test Result: Passed

เอกสารไม่ควบคุม



Chromeleon Operational Qualification, Part 3
System Suitability Test: Comparison with Expected Results

Variable Category	Report Variable	Status
System Suitability	Number	ok
	Name	ok
Test Case	Inj. Condition	ok
	Eval. Formula	ok
	Operator	ok
	Statistics	ok
	Rounding	ok
	MinimumNumberOfInjections	ok
	MaximumNumberOfInjections	ok
	Channel	ok
	Peak	ok
	Ref. Value Formula 1	ok
	Ref. Value Formula 2	ok
	N.A.	ok
System Suitability	Inj. Eval. Result	ok
	Eval. Result	ok
Test Case Result	Peak Result	ok
	Injection Condition Result	ok
	Ref. Value 1	ok
	Ref. Value 2	ok
	Result	ok
	Message	ok
	Average	ok
	Count	ok
	Maximum	ok
	Minimum	ok
	Range	ok
	Rel. Range	ok
	Rel. Std. Dev.	ok
	Std. Dev.	ok
	Sum	ok

Test Result: Passed

เอกสารไม่ควบคุม

SOFTWARE OQ



Chromeleon

Part 1 - Verification of Selected Results	PASS
Part 2 - Most Frequently Used Parameters: Comparison with Expected Results	PASS
Part 3 - System Suitability Test: comparison with Expected Results	PASS



OVERALL TEST RESULT: PASS

Field Service Representative Signature:	Customer Signature:
<i>[Signature]</i>	<i>[Signature]</i>
Date: 27/Apr/2024	Date: 22/Apr/2024

เอกสารไม่ควบคุม

PQ Anion ID#1047

Performance Qualification

TEST EQUIPMENT AND STANDARDS



Test Equipment

Equipment	Manufacturer	Model	Serial Number	Cal/Ver Date	Good Until
Multimeter	Fluke	289	27970244	N/A	N/A
Thermocouple	Fluke	K-Type	27970244	N/A	N/A
Balance	Mettler Toledo	AB204-S	1129361010	N/A	N/A
IC Qualification	Thermo Scientific	Test Box	21379153	N/A	N/A
N/A	N/A	N/A	N/A	N/A	N/A

Standards/Chemicals


Description	Manufacturer	Concentration	Part Number	Lot Number	Expiration Date
Nitrate	Thermo Scientific	5 ppm	060254	231226	Dec-2024
Nitrate	Thermo Scientific	10 ppm	060254	231226	Dec-2024
Nitrate	Thermo Scientific	25 ppm	060254	231226	Dec-2024
Nitrate	Thermo Scientific	50 ppm	060254	231226	Dec-2024
Nitrate	Thermo Scientific	100 ppm	060254	231226	Dec-2024
Nitrate	Thermo Scientific	1000 ppm	060254	231226	Dec-2024
N/A	N/A	N/A	N/A	N/A	N/A
N/A	N/A	N/A	N/A	N/A	N/A
N/A	N/A	N/A	N/A	N/A	N/A
N/A	N/A	N/A	N/A	N/A	N/A



Field Service Representative Signature:	Customer Signature:
<i>[Signature]</i>	<i>[Signature]</i>
Date: 27/Apr/2024	Date: 22/Apr/2024

เอกสารไม่ควบคุม

เอกสารไม่ควบคุม

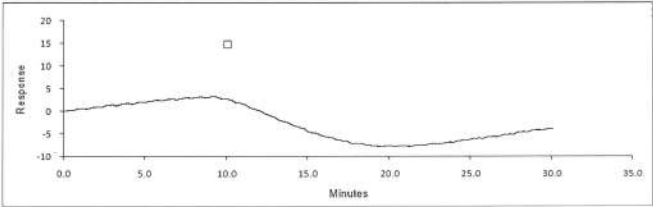

Information

System Name	Aquion RFIC
Detector SN	220360045
Data Path	chrom://desktop-c4fs317/ChromeleonLocal/Archemica/Service Contract/Validate 2024/1PM1PQ 23-04-24/Anion/IC OQ.seq/278.smp/ICD_1.channel

Noise and Drift

Test	Measured (nS)	OQ Limit (nS)	Result	Conversion Factor
Noise	1.1 nS	≤ 2.0 nS	PASS	1000
Drift	16.1 nS/hr	≤ 20.0 nS/hr	PASS	1000

OVERALL TEST RESULT: PASS



Field Service Representative Signature:	Customer Signature:
<i>K. Rattanaporn</i>	<i>Simon</i>
Date: 23/Apr/2024	Date: 23/Apr/2024

เอกสารไม่ควบคุม

Information

System Name	Aquion RFIC
Detector SN	220360045
Data Path	ChromeleonLocal://Archemica/Service Contract/Validate 2024/1PM1PQ 23-04-24/Anion/IC OQ

Peak Results

Sample Name	Injection Volume (µL)	Retention Time (min)	Area
Repeatability 01	25	0.265	2.825
Repeatability 02	25	0.265	2.822
Repeatability 03	25	0.265	2.831
Repeatability 04	25	0.265	2.835
Repeatability 05	25	0.265	2.834
Repeatability 06	25	0.265	2.836

Repeatability

Test	Measured (% RSD)	OQ Limit (% RSD)	Result
Retention Time	0.0	≤ 5.0	PASS
Area	0.2	≤ 1.0	PASS

OVERALL TEST RESULT: PASS



Field Service Representative Signature:	Customer Signature:
<i>K. Rattanaporn</i>	<i>Simon</i>
Date: 23/Apr/2024	Date: 23/Apr/2024

เอกสารไม่ควบคุม

Information

System Name	Aquion RFIC
Detector SN	220360045
Data Path	ChromeleonLocal://Archemica/Service Contract/Validate 2024/1PM1PQ 23-04-24/Anion/IC OQ

Peak Results

Sample Name	Injection Volume (µL)	Retention Time (min)	Area
Reference Blank	25	0.265	0.053
High Standard	25	0.265	49.734
Carryover	25	0.265	0.051

Results


Test	Observed (%)	OQ Limit (%)	Result
AREA	0.00	≤ 0.10	PASS

OVERALL TEST RESULT: PASS



Field Service Representative Signature:	Customer Signature:
<i>K. Rattanaporn</i>	<i>Simon</i>
Date: 23/Apr/2024	Date: 23/Apr/2024

เอกสารไม่ควบคุม

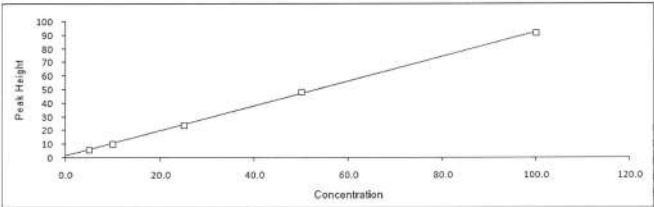

Information

System Name	Aquion RFIC
Detector SN	220360045
Data Path	ChromeleonLocal://Archemica/Service Contract/Validate 2024/1PM1PQ 23-04-24/Anion/IC OQ

Peak Results

Sample Name	Concentration	Peak Height	Calculated
Detector Linearity 01	5	5.872	4.82
Detector Linearity 02	10	10.299	9.68
Detector Linearity 03	25	23.794	24.52
Detector Linearity 04	50	48.473	51.65
Detector Linearity 05	100	91.855	99.34

Linearity

Test	Observed	OQ Limit	Result
r ²	0.999	≥ 0.999	PASS

OVERALL TEST RESULT: PASS



Field Service Representative Signature:	Customer Signature:
<i>K. Rattanaporn</i>	<i>Simon</i>
Date: 23/Apr/2024	Date: 23/Apr/2024

เอกสารไม่ควบคุม

EG Current Test

Set Point (mM)	Expected (mA)	Reading (mA)	Deviation (mA)	OQ Limit (mA)	Result
1.00	1.6082	1.604	0.00	± 0.01	PASS
5.00	8.041	8.019	0.02	± 0.05	PASS
10.00	16.082	16.037	0.05	± 0.10	PASS
50.00	80.41	80.17	0.24	± 0.50	PASS
100.00	160.82	160.32	0.50	± 1.00	PASS

OVERALL TEST RESULT: PASS



Field Service Representative Signature:	Customer Signature:
<i>K. Ruanwong</i>	<i>Simon</i>
Date: 23/Apr/2024	Date: 23/Apr/2024

เอกสารไม่ควบคุม

IC Pump Flow Rate

Set Point (mL) (mL/min)	Reading (mL/min)	Deviation (%)	OQ Limit (%)	Result
0.5	0.4995	0.100	± 2.0	PASS
1.0	0.999	0.10	± 2.0	PASS

OVERALL TEST RESULT: PASS



Field Service Representative Signature:	Customer Signature:
<i>K. Ruanwong</i>	<i>Simon</i>
Date: 23/Apr/2024	Date: 23/Apr/2024

เอกสารไม่ควบคุม

TEMPERATURE ACCURACY

Column Compartment

Set Point (°C)	Reading (°C)	Deviation (°C)	OQ Limit (°C)	Result
30.0	30.5	0.5	± 2.0	PASS

OVERALL TEST RESULT: PASS



Field Service Representative Signature:	Customer Signature:
<i>K. Ruanwong</i>	<i>Simon</i>
Date: 23/Apr/2024	Date: 23/Apr/2024

เอกสารไม่ควบคุม

OQ EXCEPTIONS AND COMMENTS

N/A

Remainder of Page Intentionally Blank

Field Service Representative Signature:	Customer Signature:
<i>K. Ruanwong</i>	<i>Simon</i>
Date: 23/Apr/2024	Date: 23/Apr/2024

เอกสารไม่ควบคุม

These Operational Qualification Results should be reviewed by the Customer. If the qualification is accepted, both the Customer and the Service Representative should sign the Operational Qualification Results, below.

OPERATIONAL QUALIFICATION RESULTS

Based upon the actual results obtained, this Operational Qualification **PASSED** the acceptance criteria described in the Operational Qualification in the Installation Checklist procedure.

Service Representative

A Field Service Representative signature below confirms the completion of all aspects of the Operational Qualification and have concluded that the system has been successfully verified to be operating as required.

Customer

A Customer signature below confirms the completion of all aspects of the Operational Qualification have been completed and that the system has been successfully verified to be operating as required.



PinAAcle 900F
Preventive Maintenance Report



Field Service Representative Signature:	Customer Signature:
<i>K. Chayanon</i>	<i>K. Chayanon</i>
Date: 23/Apr/2024	Date: 23/Apr/2024

RPG Reports v2.063
© 2024 Thermo Fisher Scientific

เอกสารไม่ควบคุม

Company Name: UAE Consultant Co., LTD.

Instrument Location: 41 Sukumvit Rd.,

Phra Khanong, Bangkok 10260

Instrument Serial No.: PFBS20031902

Date: 14-May-2024

เอกสารไม่ควบคุม

PinAAcle 900F Preventive Maintenance (PM)			
Company Name:	United Analyst and Engineering Consultant Co., LTD.		
Address (Instrument Location):	41 Sukumvit Rd., Phra Khanong, Bangkok 10260		
Serial Number:	PFBS20031902	PM Number:	2 of 2
Customer Name (if applicable):	K. Yinda	Telephone Number:	095-5580049
Customer Support Engineer Name:	K. Chayanon	Service Order Number:	WO-02787590
Date PM Performed: (DD-MMM-YYYY)	14-May-2024	Next PM Due Date: (DD-MMM-YYYY)	14-Nov-2024
Standard Labor Hours to Complete PM :		5 hours	

Part Number	Release	Publication Date	
09370145 Rev.9	A	January 2018	

Scope

The purpose of this PM is to ensure the continued functionality of the PinAAcle 900F by inspecting and replacing any worn or damaged parts. This service should only be performed by a trained representative of PerkinElmer.

The customer should save their method before the PM begins.

General Instructions:

The customer must provide the engineer operational data to demonstrate recent instrument performance prior to starting the PM.

Always check with the customer before making any changes that may affect the customer's analysis or calibration, including a current back-up of system software and/or data files.

The completed document should be signed by an authorized PerkinElmer and customer representative and left with the customer.

Update the PM sticker and instrument logbook as required.

Copyright Information

This document contains proprietary information that is protected by copyright. All rights are reserved. No part of this publication may be reproduced in any form whatsoever or translated into any language without the prior, written permission of PerkinElmer, Inc.

Copyright © 2013 PerkinElmer, Inc.

Trademarks

Registered names, trademarks, etc. used in this document, even when not specifically marked as such, are protected by law. PerkinElmer is a registered trademark of PerkinElmer, Inc. All other trademarks and registered trademarks not owned by PerkinElmer, Inc. or its subsidiaries that are depicted herein are the property of their respective owners.

Except as specifically set forth in its terms and conditions of sale, PerkinElmer makes no Warranty of any kind with regard to this document, including, but not limited to, the implied warranties of merchantability and fitness for a particular purpose.

PerkinElmer shall not be liable for incidental or consequential damages in connection with the furnishing or use of this document.

เอกสารไม่ควบคุม

Component List

Component / Specific Model	Serial #	Configuration Notes
PinAAcle900F	PFBS20031902	Syngistix V.4.0.1.1935
Fias100(New Install)	100524040501	

Parts Lists

Parts Included with the PM		
Part Number (if applicable)	Description	Quantity
B0501696	Fan Filters	N/A
N3160156	O-Ring Kits for Sampling Introduction (Stainless Steels Nebulizer)	N/A
N3160157	O-Ring Kits for Sampling Introduction (Plastic Nebulizer)	N/A
N9301714	Replacement Acetylene Filter Cartridge	N/A
TH001022	Replacement Air Filter Cartridge	N/A

Additional Reagents and Standards Required for PM

Part Number (if applicable)	Description	Quality	Batch/Lot #	Expired Date (MM/YY)
N9300183	1000 mg/L Copper Standard	AR	27-39CUY1	Apr 2025

Additional Reagents and Standards Required for PM (Customer Support Solution)

Part Number (if applicable)	Description	Quantity	Batch/Lot #	Expiration Date (MM/YY)
N/A	DI Water	250 mL	AR	AR
N/A	0.5% HNO ₃	250 mL	AR	AR

เอกสารไม่ควบคุม

Additional Tools Required for PM			
Part Number (if applicable)	Description	Quantity	Serial #
N1013000	0.2A Neutral density filter	1	101N0089015
N1013002	1.0A Neutral density filter	1	101N0089015
03030997	System 2 EDL Driver	1	03030997
N3050605	As System 2 EDL	1	16148
N3050121	Cu Lumina HCL	1	060419-030180
N3050109	Ba Lumina HCL	1	061219-020041
N3050139	K Lumina HCL	1	030819-010130
N3050152	Ni Lumina HCL	1	052719-020020

Procedure Checklist

Use (✓) to check off those steps in the checklist that have been completed.

- General:**
 - ✓ Review the instrument performance with the customer and document any recent problems.
 - ✓ Inspect the customer log book and make any appropriate PM entries.
 - ✓ Perform general inspection of system for cleanliness.
- PC Instrument Software:**
 - ✓ Instrument Software user files/databases archived, packed, and/or deleted as needed.
- Mechanical:**
 - ✓ Inspect and clean all fans and filters. Replace filters if necessary
 - ✓ Inspect all gas lines for leaks and/or wear. Replace if needed.
 - ✓ Clean exterior of the instrument.
 - ✓ Inspect the burner head, burner chamber, and nebulizer. Clean if needed as stated in the Hardware Guide.
 - ✓ Check burner head dimensions with the feeler gauge as stated in the Hardware Guide in the Maintenance chapter section on cleaning the burner head and checking sloth width. Replace if out of specification
 - ✓ Check the condition of the end cap, burner head, and nebulizer O-rings. Replace if necessary.
 - ✓ Check the drain system for signs of wear. Replace worn or damaged parts.
 - ✓ Visually check for proper flame conditions when igniting the Air-C2H2 and N2O-C2H2 flames (if applicable).
- Electrical:**
 - ✓ Inspect PC boards. Clean if necessary.
 - ✓ Carefully check all internal and external cable connections.
 - ✓ Check instrument firmware revisions upgrade to current levels (if necessary)
 - ✓ Run Diagnostics Test within the Advanced function of the Spectrometer page. Check the results in the service log folder in the Spectrometer BM Log Viewer.
- Optics:**
 - ✓ Inspect and clean the sample compartment windows, if needed.
 - ✓ Inspect optics. Clean or replace if necessary,
- Gasses:**
 - ✓ Verify that the Gasses supplied to the instrument are within the pressure and purity specifications found in the PinAAcle 900 Series Pre-installation Checklist SDB.
 - ✓ Verify that the acetylene filter and air filter element is dry. Replace if necessary.

เอกสารไม่ควบคุม

7. Flame Interlock Check:

Description: Check to ensure that all safety interlocks are closed.

Parameter	Specification	Test Results	Pass/Fail
Flame Sensor	Air/C ₂ H ₂ Flame correctly shuts down	Active	Passed
Drain Sensor	Air/C ₂ H ₂ Flame correctly shuts down	Active	Passed
Nebulizer Sensor	Air/C ₂ H ₂ Flame correctly shuts down	Active	Passed
C ₂ H ₂ Pressure Sensor	Air/C ₂ H ₂ Flame correctly shuts down	Active	Passed
Air Pressure Sensor	Air/C ₂ H ₂ Flame correctly shuts down	Active	Passed
Burner Head Sensor	Choosing Nitrous Oxide as the oxidant should trigger an interlock shuts down	Active	Passed

8. After PM Performance tests:

8.1 Detector Linearity with Barium

Description: Ensures that the detector is linear in the Visible Range.

Parameter	Specification	Certificate Value at 553.6 nm (Abs.)	Test Results	Pass/Fail
1.0 A ND Filter	± 5% from Cert.	0.9995	1.0143	Passed
0.2 A ND Filter	± 5% from Cert.	0.1936	0.1966	Passed

8.2 Baseline Noise at 1.0 Absorbance with Barium

Description: Ensures that a high absorbance will not produce excessive noise.

Parameter	Specification	Results	Pass/Fail
Standard Deviation	≤ 0.010	0.002	Passed

8.3 AA Baseline Noise with Copper

Description: Check baseline noise.

Parameter	Specification	Results	Pass/Fail
Standard Deviation	≤ 0.001	0.0002	Passed

เอกสารไม่ควบคุม

เอกสารไม่ควบคุม

8.4 D₂ Background Compensation with Copper

Description: Verifies the instruments ability to compensate for Background absorption.

Parameter	Specification	Results	Pass/Fail
Standard Deviation	≤ 0.010	0.0001	Passed

8.5 AA-BG Baseline Noise with Copper

Description: Ensures that background correction does not produce excessive noise.

Parameter	Specification	Results	Pass/Fail
Standard Deviation	≤ 0.005	0.002	Passed

8.6 AA-BG Baseline Noise with Arsenic

Description: Ensures that background correction does not produce excessive noise at a low wavelength.

Parameter	Specification	Results	Pass/Fail
Standard Deviation	≤ 0.005	0.0022	Passed

8.7 Flame Sensitivity

Description: Instrument Sensitivity checked against Copper standard.

Standard Copper Sensitivity	Specification	Results (Abs.)	Pass/Fail
5 mg/L Sensitivity SS Neb (if applicable)	> 0.250 Abs.	N/A	Not Applicable
2 mg/L Sensitivity HS Neb (if applicable)	> 0.250 Abs.	0.8005	Passed

10. Review:

- ✓ Review with the customer PM work performed.
- ✓ Review with the customer routine maintenance procedures.
- ✓ Discuss recommended customer supplied materials to have on hand.
- ✓ Attach PM sticker.

เอกสารไม่ควบคุม

Additional Comments

Additional Comments Regarding the PM

Agilent CrossLab Start Up Services

Agilent 5100 5110 ICP-OES Preventive Maintenance



Agilent Preventive Maintenance provides factory recommended service for your analytical instruments to assure reliable operation and the accuracy of your results.

Delivered by highly trained and certified service engineers using genuine Agilent parts and supplies, Agilent Preventive Maintenance provides what you need to reduce unplanned downtime and keep your systems operating at their peak performance.

This checklist is used as a guide for completing the preventive maintenance tasks. A signed copy of this checklist is provided for your records.

Review

The preventive maintenance checks and if applicable performance tests for PinAAcle 900F have been completed.

This PinAAcle 900F Passes ☒ Fails ☐ the preventive maintenance.

Review of Preventive Maintenance:

Authorized PerkinElmer Representative:	Date:
Chayanang K.	14-May-2024 (DD-MMM-YYYY)
Authorized Customer Representative:	Date:
บุญยืน หอ	14-May-2024 (DD-MMM-YYYY)

เอกสารไม่ควบคุม

เอกสารไม่ควบคุม

Introduction

Customer Information

- Customers should provide all necessary operating supplies upon request of the engineer.
- A customer representative should be available to the engineer while performing the preventive maintenance procedures. Customers are responsible for regular maintenance and are encouraged to observe the service representative.
- Any parts not included in the Parts Lists section of this document are not part of the recommended Preventive Maintenance service nor are they included in the price of this service.
- If a system requires the use of extra or special procedures and/or parts for the maintenance service, then these must be ordered separately and charged as a repair, which may incur additional costs.
- For customers using HF applications, the instrument should be returned to its standard sample introduction system.

Important Customer Web Links

- To access **Agilent University**, visit <http://www.agilent.com/crosslab/university/> to learn about training options, which include online, classroom and onsite delivery. A training specialist can work directly with you to help determine your best options.
- To access the **Agilent Resource Center** web page, visit <https://www.agilent.com/en-us/agilentresources>. The following information topics are available:
 - Sample Prep and Containment
 - Chemical Standards
 - Analysis
 - Service and Support
 - Application Workflows
- The **Agilent Community** is an excellent place to get answers, collaborate with others about applications and Agilent products, and find in-depth documents and videos relevant to Agilent technologies. Visit <https://community.agilent.com/welcome>
- Videos about specific preparation requirements for your instrument can be found by searching the **Agilent YouTube** channel at <https://www.youtube.com/user/agilent>
- Need to place a service call?** Flexible Repair Options | Agilent

เอกสารไม่ควบคุม

เอกสารไม่ควบคุม

Service Engineer's Responsibilities

- Contact the customer and ensure that all necessary supplies are available before the preventive maintenance visit.
- Only select those pages that relate to the system or module being serviced.
- Complete empty fields with the relevant information.
- Complete the relevant checkboxes in the checklist using either a "X" or tick mark "✓".
- Check "Service not applicable" check boxes to indicate services/tasks not delivered, as appropriate.
- Complete the Preventive Maintenance services in the most logical order relevant to the individual system service in the order of the tasks listed.
- Complete the **Service Review** section together with the customer.
- Complete the fields for page numbers at the foot of each selected page.
- Add relevant page numbers to selected pages and complete the total number of pages field in the Service Completion section.
- Ask the customer to sign the Service Verification section including the customer's and your signature.

Instrument Maintenance

System Information

- ☐ Check this box if an instrument configuration report is attached instead of completing the table.

Instrument System Name and ID	5110 VDV ICP-OES
Instrument System Site and Location	United Analyst and Engineering Consultant

List System Component Product Numbers	List the Serial Numbers of each Component
1. G 8059A	777 14030001
2.	
3.	
4.	
5.	
6.	
7.	
8.	
9.	

ICP-OES Configuration Table	Circle the type or write in the type if other
Nebulizer Type	SeaSpray (OneNeb) Conikal Other
Spray Chamber	Cyclonic Single Pass (Cyclonic Double Pass) Other
Torch	Radial (Dual View) Other
Torch Type	One Piece (Semi Demountable) Fully Demountable Other
Injector Diameter	2.4mm (1.8mm) 1.4mm 0.8mm Other
Injector Material	Quartz Ceramic Other

Preparation

- ☒ Discuss any specific issues with the customer before starting.
- ☒ Review the instrument logbook for recorded problems and comments.
- ☒ Save instrument control settings before starting the procedure.
- ☒ Perform a general inspection of the system for cleanliness.
- ☒ Check for proper installation of parts, assemblies, sensors etc.
- ☒ Check system for required installation of components and implementation of Service Notes
- ☒ Check for required firmware/software updates and verify with customers if they would like them installed.
- ☐ For HF application systems, if standard sample introduction system was not installed, ask the customer to install it. (11/1)
- ☒ Ask the customer to remove any samples from the ICP-OES sample introduction area, auto sampler or around the ICP-OES.

Preventive Maintenance Procedures

Record Pre-PM instrument performance

- ☒ Run Instrument Performance test.
- ☒ Record results in Instrument Performance Test Results Table – Pre-PM.

Clean and inspect ICP-OES system

- ☒ Look for any obvious external damage or problems.
- ☒ Inspect water cooling hoses, gas lines and power cord for excessive wear or damage.
- ☒ Perform a general internal inspection of the system for excessive dust accumulation, clean if necessary.
- ☒ Inspect sample introduction components and record any required maintenance in the Service Engineer Comments and notify the customer as the required actions required.
- ☒ Record the instrument operating conditions in the ICP-OES Status Results Table.
- ☒ Replace the polychromator purge filter.
- ☒ Replace the radial pre-optics window
- ☒ Replace the axial pre-optics window for SVDV and VDV instruments.
- ☒ Check exhaust flow for the correct positive extraction at the exhaust duct to insure they meet minimum specifications.
- ☒ Replace air inlet dust filter.
- ☐ Replace high capacity air inlet dust filter element if installed. (11/1)
- ☒ Remove and clean instrument water inlet filter.

Agilent Water Recirculator

- ☐ Service not applicable
- ☒ Drain cooling fluid and remove any particles from the chiller reservoir
- ☒ Remove, clean and reinstall water inlet metal mesh filter if present.
- ☒ Re fill with Agilent Cool Clear cooling fluid.
- ☒ Clean the cooling system Air filter and the condenser.

SPS 3 Auto Sampler

- ☒ **Service not applicable**
- ☐ Power cycle the autosampler and verify successful initialization.
- ☐ Inspect X and Z axis belts for wear. Replace is necessary.
- ☐ Clean X and Z axis slide shafts.
- ☐ Using customer's racks and the Agilent software move the sample probe to the 4 outermost corners and rinse port, ensure that the probe is approximately centered in the vial.

SPS 4 Auto sampler

- ☒ **Service not applicable**
- ☐ Clean the spill tray, rack location mat, end frames and chassis with a damp soft cloth and diluted mild detergent.
- ☐ Clean the auto sampler cover panels, if cover kit is installed, with domestic window cleaner.
- ☐ Check the X-axis and Z-axis drive belts for cracks, splits, damaged teeth, excessive fraying, color changes or degradation from fumes.
- ☐ Check the X-axis, Theta-axis and Z-axis FFC cables for cracks, incorrect positioning, damaged edges or damaged connectors.
- ☐ Pump Tubing Replacement. Replace peristaltic pump tubing. Replace all tubing that goes from the rinse station to the pump and from the pump to the waste/rinse bottles
- ☐ Test using customer's tray and move the sample probe to the sample vial 1, wash vial and rinse port and ensure that the probe is centered in the vial. If not use calibration wizard and calibrate the position.

AVS 4, 6, 7 Advanced Valve System

- ☒ **Service not applicable**
- ☐ Replace valve rotor seal
- ☐ Check fittings for signs of leaks
- ☐ Check tubing including autosampler tubing for kinks or excessive wear
- ☐ Check high flow pump for signs of leaks

ICP-OES adjustment

- ☒ Check position of Zn peak, adjust if required.
- ☒ Check Argon Ratio, adjust to specified value if required.
- ☒ Perform Detector Calibration.
- ☒ Perform Instrument Calibration.

Record Post-PM instrument performance

- ☒ Run Instrument Performance test.
- ☒ Record results in Instrument Performance Test Results Table - Post PM.
- ☒ For systems using ICP Expert version 7.3 and above, run the following Instrument tests
 - ☒ Subsystem Communications Test
 - ☒ Air Flow
 - ☒ Water Flow
 - ☒ Gas Flows
 - ☒ RF Generator
 - ☒ Camera Test
 - ☒ Optics Test
 - ☒ Nebulizer Test

- ☒ Record the result in the Instrument Test Results Table

Restore Instrument

- ☐ For HF applications, ask the customer to reinstall their sample introduction system. N/A
- ☒ Leave system in an idle state: on and purging.
- ☒ Guidance: If the PM service is performed prior to a qualification service, then use the qualification procedure as a guide for final instrument set up and checkout.

Service Review

- ☒ Attach available reports/printouts of all tests to this documentation.
- ☒ Record the Preventive Maintenance service activity in the customer's records/logbook.
- ☒ Record the PM event in the Smart Alerts logbook, if applicable.
- ☒ Update/reset instrument maintenance counters as appropriate.
- ☒ Affix the PM sticker to the system or instrument logbook based on the customer's request.
- ☒ Complete the Service Engineer Comments section if there are additional comments.
- ☒ Review this service, parts replaced, and test results obtained with the customer.
- ☒ If the instrument firmware was updated, record the details of the change in the Service Engineer's Comments box. Systems in a compliant environment may need additional documentation.
- ☒ Complete the Signature Page with both Service Engineer and Customer signatures.

Test Results**Instrument Performance Test Results Table**

Note: These measurements do not form part of any specification and are for reference only.

	Pre PM Sensitivity Check		Post PM Sensitivity Check	
	Radial	Axial *	Radial	Axial*
Zn 213.857 nm SRBR	1500.9	2219.4	4124.9	6965.9
Mn 257.610 nm SRBR	3915.0	7492.2	13017.6	31121.6
Al 396.152 nm SBR	9.7	10.7	9.7	21.1
K 766.491 nm SBR	6.7	28.1	4.8	45.3

* Axial result is not applicable for G8016AA, G8012AA Radial View instruments.

Instrument Test Results Table

Note: The Instrument Test results are for systems using ICP Expert version 7.3 and above only.

Instrument Test	Result
Subsystem Communications Test	Pass
Air Flow	Pass
Water Flow	Pass
Gas Flows	Pass
RF Generator	Pass
Camera Test	Pass
Optics Test	Pass
Nebulizer test	Pass

ICP-OES Status Results Table

Note: These measurements do not form part of any specification and are for reference only.

Measurement	Standby Mode	Plasma On
Mains Voltage	231.411 VAC	226.831 VAC
Mains Current	0.051 A	0.105 A
Instrument Temperature	22.1 °C	23.5 °C
RF Air Flow (sensor speed)	14.0 Hz	19.0 Hz
Plasma Exhaust Temperature	No measurement	63.6 °C
Water Flow Oscillator	No measurement	1.34 L/min
Water Flow Detector	0.86 L/min	0.81 L/min
Water Inlet Temperature	19.3 °C	19.3 °C
Polychromator Temperature	35.0 °C	35.0 °C
CCD Temperature	-40.1 °C	-39.6 °C
Thermal Stabilizer	35.0 °C	35.0 °C
Argon Supply Pressure	646.92 kPa	591.55 kPa
Purge Gas Supply Pressure*1	646.66 kPa	612.41 kPa
Option Gas Supply Pressure*1	— kPa	— kPa
Nebulizer Flow	No measurement	0.30 L/min
Nebulizer Back Pressure	No measurement	158.43 kPa
Plasma Gas Flow	No measurement	11.91 L/min
Auxiliary Gas Flow	No measurement	1.00 L/min
RF Power	No measurement	1204.3 W
RF Supply Current	No measurement	3.856 A
RF Supply Voltage	No measurement	204.417 V

*1 If option installed

Consumed PM Parts

Part Description	Part Number	Product or Model# where used	Quantity consumed
Axial Pre-Optic Window	G8010-68014	G8010A, G8011A, G8014A/G8015A	1
Radial Pre-Optic Window	G8010-68015	All	1
Agilent Cool Clear Coolant Fluid	5799-0037	Agilent Water Recirculator	—
Purge Gas Filter	G8010-60136	All	1
Air inlet filter	G8000-68002	All	1
High Capacity Air Filter	G8010-60189	Optional	—
Rotor seal for 6-7 port valve for AVS6/7	G8494-60002	G8494A/G8495	—
Rotor seal for 4 port valve for AVS4	G8493-60002	G8493A	—
Rinse solution to rinse station 2.5mm id x 1m	G8410-80123	SPS 4	—
Barb connector 2.5mm-1.5mm ID	G8410-80124	SPS 4	—
PVC waste tubing, 8mm od x 5mm id, 2m	G8410-80122	SPS 4	—
Additional Parts may be required from engineer's stock:			
X axis drive belt	5410047500	SPS 3	—
Z axis drive belt	5410047400	SPS 3	—
Peristaltic pump tubing, PVC SolvaFlex, 3 bridged,	3710049000	SPS 4	—

Consumed Parts Reference
(Purchased by customer, not included as part of PM)☒ Section Not Applicable.

Part Description	Part Number	Product or Model# where used	Quantity consumed

Signature Page

Service Engineer Comments (optional)

If there are any specific points you wish to note as part of performing the installation or other items of interest for the customer, please write in this box.

Service Verification

Service Request Number:

6003193100

Service Engineer Name:

Kanyakorn S.

Service Engineer Signature:

Kanyakorn S.

Total number of pages in this document:

14

Date Service Completed:

04 Nov 2024

Customer Name:

Aphorn Onkong

Customer Signature:

Aphorn Onkong

Report Summary

Instrument Model	Agilent 5100/5110 VDV ICP-OES
Instrument ID	G8011A/G8015A
Instrument Serial Number	MY18030001
Software Version	7.3.1.9507
Firmware Version	3442
Tested By	Pre Test_PM_Kanyakorn S.
Test Completed On	11/4/2024 9:19:10 AM

Result Summary

Subsystem Communications Test	Skipped
Air Flow Test	Skipped
Water Flow Test	Skipped
Gas Flows Test	Skipped
RF Generator Test	Skipped
Camera Test	Skipped
Optics Test	Skipped
Advanced Valve System Test	Skipped
Resolution Test	Pass
Sensitivity Test	Fail
Precision Test	Pass

Resolution Test			Pass
Element Wavelength	Specification	Width	
N (174.213 nm)	≤ 9.40	6.98	
As (188.980 nm)	≤ 8.20	6.17	
C (193.027 nm)	≤ 11.50	8.30	
Mo (202.032 nm)	≤ 8.20	6.38	
Cr (206.158 nm)	≤ 13.40	8.98	
Zn (213.857 nm)	≤ 8.70	6.60	
Pb (220.353 nm)	≤ 9.50	7.09	
Co (228.615 nm)	≤ 17.20	11.67	
Ba (230.424 nm)	≤ 9.40	7.20	
Mn (257.610 nm)	≤ 13.30	9.43	
Mn (260.568 nm)	≤ 20.30	14.11	
Cr (267.716 nm)	≤ 11.00	8.04	
Cu (324.754 nm)	≤ 25.00	18.97	
Cu (327.395 nm)	≤ 14.20	11.23	
Sr (338.071 nm)	≤ 33.50	24.30	
Ba (455.403 nm)	≤ 44.00	33.47	
Sr (460.733 nm)	≤ 36.00	17.23	
Ba (493.408 nm)	≤ 36.00	25.37	
Ba (614.171 nm)	≤ 42.00	25.54	
Ar (675.283 nm)	≤ 74.00	56.51	
K (766.491 nm)	≤ 80.00	65.86	

Page 2 of 4

เอกสารไม่ควบคุม

Sensitivity Test			Fail		
Radial					
Element Wavelength	Specification	Method	Ratio	Standard	Blank
As (188.980 nm)	≥ 46.0	SRBR	104.1	793.0	50.8
Se (196.026 nm)	≥ 41.0	SRBR	87.6	862.0	79.7
Zn (213.857 nm)	≥ 1421.0	SRBR	1500.8	41823.3	749.0
Pb (220.353 nm)	≥ 46.0	SRBR	170.7	2432.0	174.9
Mn (257.610 nm)	≥ 3518.0	SRBR	3915.0	264700.2	4420.0
Al (396.152 nm)	≥ 3.4	SBR	7.7	48454.6	5563.2
Ba (493.408 nm)	≥ 34.0	SBR	45.9	1966719.7	41903.8
K (766.491 nm)	≥ 1.8	SBR	5.7	99038.2	14687.7
Axial					
Element Wavelength	Specification	Method	Ratio	Standard	Blank
As (188.980 nm)	≥ 208.0	SRBR	126.5	1498.8	119.0
Se (196.026 nm)	≥ 159.0	SRBR	112.0	1773.6	197.8
Zn (206.200 nm)	≥ 234.0	SRBR	466.0	6784.2	199.7
Zn (213.857 nm)	≥ 1743.0	SRBR	2217.4	95597.6	1789.7
Cd (214.439 nm)	≥ 4227.0	SRBR	1919.3	68724.6	1236.4
Pb (220.353 nm)	≥ 320.0	SRBR	332.6	7929.5	499.0
Mn (257.610 nm)	≥ 10625.0	SRBR	7492.2	991238.3	16911.7
Cr (267.716 nm)	≥ 1048.0	SRBR	2254.6	129706.6	3150.9
Cu (324.754 nm)	≥ 19.0	SBR	26.9	290746.3	10407.5
Al (396.152 nm)	≥ 6.0	SBR	10.7	211329.2	18005.0
Ba (493.408 nm)	≥ 60.0	SBR	49.3	6956460.4	138336.9
K (766.491 nm)	≥ 24.0	SBR	28.1	1395190.2	47996.2

Page 3 of 4

เอกสารไม่ควบคุม

Precision Test			Pass
Radial			
Element Wavelength	Specification	Measured Value % RSD	
As (188.980 nm)	≤ 2.60	0.73	
Se (196.026 nm)	≤ 2.60	0.95	
Zn (213.857 nm)	≤ 1.50	0.31	
Pb (220.353 nm)	≤ 2.60	0.73	
Mn (257.610 nm)	≤ 1.50	0.39	
Al (396.152 nm)	≤ 1.50	0.39	
Ba (493.408 nm)	≤ 1.50	0.87	
K (766.491 nm)	≤ 1.50	0.32	
Axial			
Element Wavelength	Specification	Measured Value % RSD	
As (188.980 nm)	≤ 1.50	1.21	
Se (196.026 nm)	≤ 1.50	0.84	
Zn (206.200 nm)	≤ 1.50	0.56	
Zn (213.857 nm)	≤ 1.50	0.96	
Cd (214.439 nm)	≤ 1.50	0.26	
Pb (220.353 nm)	≤ 1.50	0.51	
Mn (257.610 nm)	≤ 1.50	0.97	
Cr (267.716 nm)	≤ 1.50	0.22	
Cu (324.754 nm)	≤ 1.50	0.24	
Al (396.152 nm)	≤ 1.50	0.33	
Ba (493.408 nm)	≤ 1.50	0.40	
K (766.491 nm)	≤ 1.50	0.65	

Page 4 of 4

เอกสารไม่ควบคุม

Report Summary	
Instrument Model	Agilent 5100/5110 VDV ICP-OES
Instrument ID	G8011A/G8015A
Instrument Serial Number	MY18030001
Software Version	7.3.1.9507
File Name	3442
Tested By	Post Test_PM_Kanyakorn S.
Test Completed On	11/4/2024 11:07:24 AM
Result Summary	
Subsystem Communications Test	Pass
Air Flow Test	Skipped
Water Flow Test	Skipped
Gas Flows Test	Skipped
RF Generator Test	Skipped
Camera Test	Skipped
Optics Test	Pass
Advanced Valve System Test	Skipped
Resolution Test	Pass
Sensitivity Test	Fail
Precision Test	Pass
Subsystem Communications Test	Pass
Optics Test	Pass
Intensity	3184054
Wavelength	737.212
	3177175
	737.212

Page 1 of 4

เอกสารไม่ควบคุม

Resolution Test			Pass
Element Wavelength	Specification	Width	
N (174.213 nm)	≤ 9.40	6.97	
As (188.980 nm)	≤ 8.20	6.14	
C (193.027 nm)	≤ 11.50	8.33	
Mo (202.032 nm)	≤ 8.20	6.33	
Cr (206.133 nm)	≤ 13.40	9.06	
Zn (213.637 nm)	≤ 8.70	6.70	
Pb (220.353 nm)	≤ 9.50	7.03	
Co (228.615 nm)	≤ 17.20	11.72	
Ba (230.424 nm)	≤ 9.40	7.32	
Mn (257.610 nm)	≤ 13.30	9.44	
Mn (260.568 nm)	≤ 20.30	14.21	
Cr (267.716 nm)	≤ 11.00	7.94	
Cu (324.754 nm)	≤ 25.00	18.99	
Cu (327.395 nm)	≤ 14.20	11.27	
Sr (338.071 nm)	≤ 33.50	24.40	
Ba (455.403 nm)	≤ 44.00	33.50	
Sr (460.733 nm)	≤ 36.00	17.31	
Ba (493.408 nm)	≤ 36.00	25.44	
Ba (614.171 nm)	≤ 42.00	25.16	
Ar (675.283 nm)	≤ 74.00	56.15	
K (766.491 nm)	≤ 80.00	65.56	

Page 2 of 4

เอกสารไม่ควบคุม

Sensitivity Test			Fail		
Radial					
Element Wavelength	Specification	Method	Ratio	Standard	Blank
As (188.980 nm)	≥ 46.0	SRBR	130.6	977.1	50.4
Se (196.026 nm)	≥ 41.0	SRBR	106.0	958.7	70.2
Zn (213.857 nm)	≥ 1421.0	SRBR	4124.8	44037.7	113.4
Pb (220.353 nm)	≥ 46.0	SRBR	207.2	2554.7	136.2
Mn (257.610 nm)	≥ 3518.0	SRBR	13017.8	271846.6	434.7
Al (396.152 nm)	≥ 3.4	SBR	9.7	50615.5	4717.0
Ba (493.408 nm)	≥ 34.0	SBR	133.7	2069203.0	15359.3
K (766.491 nm)	≥ 1.8	SBR	4.8	100199.5	17235.5
Axial					
Element Wavelength	Specification	Method	Ratio	Standard	Blank
As (188.980 nm)	≥ 208.0	SRBR	174.9	1566.7	73.0
Se (196.026 nm)	≥ 159.0	SRBR	167.0	1863.4	110.2
Zn (206.200 nm)	≥ 234.0	SRBR	740.9	6836.0	83.1
Zn (213.857 nm)	≥ 1743.0	SRBR	6965.9	101568.1	211.7
Cd (214.439 nm)	≥ 4227.0	SRBR	5781.0	72852.9	158.1
Pb (220.353 nm)	≥ 320.0	SRBR	501.0	8464.3	267.7
Mn (257.610 nm)	≥ 10625.0	SRBR	31121.6	1006637.8	1044.0
Cr (267.716 nm)	≥ 1048.0	SRBR	4424.8	132202.9	880.8
Cu (324.754 nm)	≥ 19.0	SBR	68.7	302907.8	4345.6
Al (396.152 nm)	≥ 6.0	SBR	21.1	218771.0	9892.3
Ba (493.408 nm)	≥ 60.0	SBR	250.6	7137380.9	28367.3
K (766.491 nm)	≥ 24.0	SBR	45.3	1435050.6	31025.0

Page 3 of 4

เอกสารไม่ควบคุม

Precision Test			Pass
Radial			
Element Wavelength	Specification	Measured Value % RSD	
As (188.980 nm)	≤ 2.60	0.81	
Se (196.026 nm)	≤ 2.60	0.98	
Zn (213.857 nm)	≤ 1.50	0.22	
Pb (220.353 nm)	≤ 2.60	0.37	
Mn (257.610 nm)	≤ 1.50	0.27	
Al (396.152 nm)	≤ 1.50	0.25	
Ba (493.408 nm)	≤ 1.50	0.53	
K (766.491 nm)	≤ 1.50	0.15	
Axial			
Element Wavelength	Specification	Measured Value % RSD	
As (188.980 nm)	≤ 1.50	0.81	
Se (196.026 nm)	≤ 1.50	0.65	
Zn (206.200 nm)	≤ 1.50	0.79	
Zn (213.857 nm)	≤ 1.50	0.81	
Cd (214.439 nm)	≤ 1.50	0.35	
Pb (220.353 nm)	≤ 1.50	0.33	
Mn (257.610 nm)	≤ 1.50	1.02	
Cr (267.716 nm)	≤ 1.50	0.32	
Cu (324.754 nm)	≤ 1.50	0.51	
Al (396.152 nm)	≤ 1.50	0.37	
Ba (493.408 nm)	≤ 1.50	0.68	
K (766.491 nm)	≤ 1.50	0.74	

Page 4 of 4

เอกสารไม่ควบคุม

Report Summary		
Instrument Model	Agilent 5100/5110 VDV ICP-OES	
Instrument ID	G8011A/G8015A	
Instrument Serial Number	MY18030001	
Software Version	7.3.1.9507	
Firmware Version	3442	
Tested By	Post Test_PM_Kanyakorn S.	
Test Completed On	11/4/2024 11:30:15 AM	
Result Summary		
Subsystem Communications Test	Pass	
Air Flow Test	Pass	
Water Flow Test	Pass	
Gas Flows Test	Pass	
RF Generator Test	Pass	
Camera Test	Pass	
Optics Test	Skipped	
Advanced Valve System Test	Skipped	
Resolution Test	Skipped	
Sensitivity Test	Skipped	
Precision Test	Skipped	
Subsystem Communications Test	Pass	
Air Flow Test	Pass	
30% Air Flow (relative speed)	75% Air Flow (relative speed)	
15.00	19.00	
Water Flow Test	Pass	
RF Water Flow(L/min)	Camera Water Flow (L/min)	Water Inlet Temperature (°C)
1.30	0.81	20.55

Page 1 of 2

เอกสารไม่ควบคุม

Gas Flows Test					
Pass					
Nebulizer Target Flow	Actual Flow	Back Pressure	Auxiliary Target Flow	Actual Flow	Back Pressure
0.70	0.70	154.65	2.00	2.00	110.92
Makeup Target Flow	Actual Flow	Back Pressure	Plasma Target Flow	Actual Flow	Back Pressure
2.00	2.00	115.38	18.00	17.97	21.48
RF Generator Test					
Pass					
RF Power Supply Test	Passed				
RF Power Supply (V)	128.554				
RF Oscillator Test	Passed				
RF Oscillator Frequency (MHz)	25.834				
Work Coil Current (A)	44.660				
RF Power Supply Current (A)	1.999				
Camera Test					
Pass					
	Integration Time (ms)	Standard Deviation	Status		
Electronic Offset Test	1000	5.228	Passed		
Dark Current Test	6000	1.168	Passed		
Array Test	5	0.024	Passed		
Linearity Test		0.118	Passed		

Page 2 of 2

เอกสารไม่ควบคุม

Report Summary	
Instrument Model	Agilent 5100/5110 VDV ICP-OES
Instrument ID	G8011A/G8015A
Instrument Serial Number	MY18030001
Software Version	7.3.1.9507
Firmware Version	3442
Tested By	change mirror
Test Completed On	11/6/2024 10:35:26 AM
Result Summary	
Subsystem Communications Test	Skipped
Air Flow Test	Skipped
Water Flow Test	Skipped
Gas Flows Test	Skipped
RF Generator Test	Skipped
Camera Test	Skipped
Optics Test	Skipped
Advanced Valve System Test	Skipped
Resolution Test	Pass
Sensitivity Test	Pass
Precision Test	Pass

Page 1 of 4

เอกสารไม่ควบคุม

Resolution Test		
Pass		
Element Wavelength	Specification	Width
N (174.213 nm)	≤ 9.40	6.79
As (188.980 nm)	≤ 8.20	5.80
C (193.027 nm)	≤ 11.50	8.15
Mo (202.032 nm)	≤ 8.20	5.90
Cr (206.158 nm)	≤ 13.40	8.85
Zn (213.857 nm)	≤ 8.70	6.77
Pb (220.353 nm)	≤ 9.50	6.61
Co (228.615 nm)	≤ 17.20	11.79
Ba (230.424 nm)	≤ 9.40	7.25
Mn (257.610 nm)	≤ 13.30	9.47
Mn (260.568 nm)	≤ 20.30	14.50
Cr (267.716 nm)	≤ 11.00	7.91
Cu (324.754 nm)	≤ 25.00	18.72
Cu (327.395 nm)	≤ 14.20	11.09
Sr (338.071 nm)	≤ 33.50	25.39
Ba (455.403 nm)	≤ 44.00	33.09
Sr (460.793 nm)	≤ 36.00	18.54
Ba (493.408 nm)	≤ 36.00	25.74
Ba (614.171 nm)	≤ 42.00	25.23
Ar (675.283 nm)	≤ 74.00	58.92
K (766.491 nm)	≤ 80.00	63.16

Page 2 of 4

เอกสารไม่ควบคุม

Sensitivity Test					
Pass					
Radial					
Element Wavelength	Specification	Method	Ratio	Standard	Blank
As (188.980 nm)	≥ 46.0	SRBR	110.5	868.9	54.3
Se (196.026 nm)	≥ 41.0	SRBR	88.3	934.7	91.3
Zn (213.857 nm)	≥ 1421.0	SRBR	3535.4	44017.7	153.9
Pb (220.353 nm)	≥ 46.0	SRBR	184.5	2492.3	159.8
Mn (257.610 nm)	≥ 3518.0	SRBR	11099.6	249595.3	503.6
Al (396.152 nm)	≥ 3.4	SBR	8.7	50274.4	5172.0
Ba (493.408 nm)	≥ 34.0	SBR	124.5	1903164.1	15166.0
K (766.491 nm)	≥ 1.8	SBR	6.9	110041.4	13991.2
Axial					
Element Wavelength	Specification	Method	Ratio	Standard	Blank
As (188.980 nm)	≥ 208.0	SRBR	253.3	3744.3	196.3
Se (196.026 nm)	≥ 159.0	SRBR	206.7	4199.7	347.2
Zn (206.200 nm)	≥ 234.0	SRBR	923.0	12282.3	172.1
Zn (213.857 nm)	≥ 1743.0	SRBR	6398.3	157551.5	601.7
Cd (214.439 nm)	≥ 4227.0	SRBR	5069.2	99873.7	385.2
Pb (220.353 nm)	≥ 320.0	SRBR	389.0	10641.1	658.6
Mn (257.610 nm)	≥ 10625.0	SRBR	21190.4	985528.7	2153.6
Cr (267.716 nm)	≥ 1048.0	SRBR	3054.1	131797.6	1811.5
Cu (324.754 nm)	≥ 19.0	SBR	36.3	301401.4	8082.9
Al (396.152 nm)	≥ 6.0	SBR	10.8	228359.5	19280.5
Ba (493.408 nm)	≥ 60.0	SBR	106.5	6460421.5	60122.8
K (766.491 nm)	≥ 24.0	SBR	30.2	1639840.6	52562.1

Page 3 of 4

เอกสารไม่ควบคุม

Calibration Certificate

Certificate No.: 2401718-001-01
Client name: UNITED ANALYST AND ENGINEERING CONSULTANT CO., LTD.
Address: 3 Soi Udomsuk 41, Sukhumvit Road,
Bangchack, Prakhong, Bangkok 10260

Page 1 of 5

Equipment: pH Meter
Manufacturer: METTLER TOLEDO
Model: SevenEasy pH
Serial No.: 1231155210
ID No.: UAE.WAT.010/2553
Order No.: 2401718
Operation No.: 2401718-001
Date of Receipt: 27 February 2024
Date of Calibration: 11 March 2024

Calibrated by Mr. Manas Somsak Specialist
Approved by (Mr. Pheraphat Tuanjit)
Manager, Division of Calibration Laboratory
Responsible for the Technical Management Team
Date of Issue: 12 March 2024

The uncertainties are for a confidence probability of approximately 95%.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the National Food Institute.

F-CS-009 Revision: 01 Date: 20-04-65

Calibration Report

Certificate No.: 2401718-001-01
Equipment: pH Meter
Resolution: 0.01 pH ; 1 mV
Manufacturer: METTLER TOLEDO
Model: SevenEasy pH
Serial No.: 1231155210
Type: Bench top
ID No.: UAE.WAT.010/2553
Date of Calibration: 11 March 2024

Location: Chemical Calibration Laboratory, National Food Institute
Environment Condition: Ambient Temperature: (23.4 ± 1.5) °C Relative Humidity: (51 ± 3) %
Condition of Equipment: Good Condition
Condition of this Results of Calibration

1. Calibration Method W-CC-002 : In house method based on direct measurement by using standard voltage calibrator and certified reference material (CRM)

2. Reference Standards / Certified Reference Material

Instruments	Serial / ID No.	Manufacturer	Certificate No.	Due Date	
2.1 DC Voltage Calibrator	2709007	Fuke	23E2003	14 June 2024	
2.2 Digital Thermometer	2709007	Fuke	CC 660570-01	30 October 2024	
2.3 Thermo-Hygro Meter	NFLBTH 01423	testo	CC 660353-01	3 April 2024	
Certified Reference Material		Lot. No.	Manufacturer	Ref. N	Expire Date
2.4 pH buffer 4.006 (Primary pH buffer Solution)	888842	CPAchem	PH216.L5	13 April 2025	
2.5 pH buffer 6.865 (Primary pH buffer Solution)	888843	CPAchem	PH217.L5	13 April 2025	
2.6 pH buffer 10.01 (Primary pH buffer Solution)	888844	CPAchem	PH220.L5	13 April 2024	
2.7 pH buffer 7.00 (Standard pH buffer Solution)	C03109	HACH LANGE GmbH	S11M004	18 October 2025	

3. This certification is traceable to The International System of Unit (SI Unit)

- 3.1 Instruments Ng.2.1 through NSC-TISI-TIS 17025 Laboratory Accreditation of Calibration No.0008
3.2 Instruments Ng.2.2 and 2.3 through NSC-TISI-TIS 17025 Laboratory Accreditation of Calibration No.0061
3.3 Certified Reference Material Ng.2.4 to 2.6 traceable to Primary measurement method: Harned cell using calibrated thermometer, barometer, and nanovoltmeter. The Standard Solution preparation and certified by CPAchem Ltd is accredited to ISO 17034 and ISO/IEC 17025
3.4 Certified Reference Material Ng.2.7 traceable to PTB Certificate Nr. PTB-PHQA-563/30504/23 and Certificate Nr. PTB-PHOB-565/30620/22 (PTB Physikalisch-Technische Bundesanstalt, Braunschweig, Germany)

4. This certificate was certified only for the instrument we calibrated.

5. This result of calibration was found accurate as shown on date and place of calibration only.

F-CS-012 Revision: 01 Date: 20-04-65

เอกสารไม่ควบคุม

Calibration Report

Certificate No.: 2401718-001-01
Equipment: pH Meter
Resolution: 0.01 pH ; 1 mV
Manufacturer: METTLER TOLEDO
Model: SevenEasy pH
Serial No.: 1231155210
Type: Bench top
ID No.: UAE.WAT.010/2553
Date of Calibration: 11 March 2024

Calibration Results: (Manual Temperature Compensation at 25 °C)

1. Calibration of pH Meter (offset value before adjust: -0.4 mV)

Nominal pH	DC Voltage Standard (mV)	Average Indicator Reading		Uncertainty (±mV)	Coverage Factor (k)
		mV	pH		
0	414.121	414	0.00	0.58	2.00
2	295.814	296	2.00	0.58	2.00
4	177.464	178	4.00	0.58	2.00
6	59.160	59	6.00	0.58	2.00
7	0.001	0	7.00	0.58	2.00
8	-59.159	-59	8.00	0.58	2.00
10	-177.461	-177	10.00	0.58	2.00
12	-295.811	-296	12.00	0.58	2.00
14	-414.118	-414	14.00	0.58	2.00

2. Calibration of pH Meter with Electrode (Manual Temperature Compensation at 25 °C)

Equipment: pH Electrode Type: Combined Electrode
Manufacturer: METTLER TOLEDO Model: InLab Solids
Serial No.: 3060701 ID No: N/A
Performance of Electrode system (Three-Point Calibration at pH 4, 7 and 10)

Certified Value @25 °C (pH)	Average Indicator Reading		Relative Slope (%)	Uncertainty (± pH)	Coverage Factor (k)
	pH	mV			
4.008	4.01	188	-	0.0071	2.00
7.001	7.00	13	98.9	0.0086	2.00
10.010	10.01	-160	97.2	0.0085	2.00
6.865	6.87	21	-	0.0074	2.00

F-CS-012 Revision: 01 Date: 20-04-65

เอกสารไม่ควบคุม

เอกสารไม่ควบคุม

Calibration Report

Certificate No.: 2401718-001-01
Equipment: Digital Thermometer with RTD (pH Meter)
Resolution: 0.1 °C Model: SevenEasy pH
Serial No.: 1231155210 ID No.: UAE.WAT.010/2553
Manufacturer: METTLER TOLEDO
Date of Calibration: 11 March 2024 Page 4 of 5

Location: Chemical Calibration Laboratory, National Food Institute
Environment Condition: Ambient Temperature 23 °C ± 1 °C
Relative Humidity 51 % ± 2 %

Condition of this results of Calibration:

- Calibration Method:
 - In house method: W-TE-025 by comparison with standard thermometer.
 - The Calibration is determined by comparing with a known temperature from a standard resistance thermometer.
 - The temperature scale in use at this laboratory is the International Temperature scale of 1990 (ITS-90).

2. Reference Standard Instrument:


Instrument	Model	Serial No.	Certificate No.	Due Date	Through
HANDHELD THERMOMETER	1523	2116154	PSL-T 087766	06-Jun-24	TISTR
Platinum Resistance Thermometer (PRT)	5627A	877332			

Support Equipment: - Low Temperature Bath (ISOCAL-6), Model: Europa-6 Plus Basic, S/N: 341592/2

- This certificate is traceable to International System of Units (SI Units).
- This certificate was certified only for the instrument we calibrated.
- This result of calibration was found accurate as shown on date and place of calibration only.

Condition of Calibrated item: Good
Result of Calibration: ☒ Without adjustment ☐ After adjustment

F-CS-012 Revision: 01 Date: 20-04-65



Calibration Report

Certificate No.: 2401718-001-01
Equipment: Digital Thermometer with RTD (pH Meter)
Resolution: 0.1 °C Model: SevenEasy pH
Serial No.: 1231155210 ID No.: UAE.WAT.010/2553
Manufacturer: METTLER TOLEDO
Date of Calibration: 11 March 2024 Page 5 of 5

Calibration point: 15.0, 25.0 and 35.0 °C
Calibration result:

- The probe was immersed in liquid bath or dry bath to a minimum depth of 100 mm.
- Description of probe, model: N/A S/N: N/A
- Dimension of probe: Diameter: 4 mm, Length: 120 mm.
- Sheath material: Stainless Steel

UUC* Reading (°C)	Standard Temperature (°C)	Correction Value (°C)	Uncertainty ± (°C)
15.1	14.998	0.1	0.099
25.1	24.998	0.1	0.099
35.1	34.997	0.1	0.099


Note

- UUC*: Unit Under Calibration

The report uncertainty of measurement was based on standard uncertainty multiplied by coverage factor k=2, providing a level of confidence of approximately 95 %.

----- End -----

F-CS-012 Revision: 01 Date: 20-04-65



Certificate of Calibration

Equipment: pH METER Certificate No.: C07240167
Model: SevenEasy Issued Date: 9 April 2024
Serial No. (or ID.): 1230525212 (UAE.WAS.003/2553) Job No.: WO-0002408
Manufacturer: METTLER TOLEDO Page: 1 of 3
Electrode Serial No.: 1156883 Model: InLab Solids Brand: METTLER TOLEDO
Condition: In Condition

Customer: United Analyst and Engineering Consultant Company Limited
3 Soi Udomsuk 41 Sukhumvit Road,
Bangkok, Prakanong, Bangkok 10260 Thailand

Environment Condition: Temperature 23 °C ± 2 °C
Humidity 50 %RH ± 15 %RH

Calibration Place: Environment Laboratory, DKSH Technology Limited,
2533 Sukhumvit Road, Bangkok,
Phrakhanong, Bangkok 10260 Thailand

Calibration By: Miss.Orawan Khlaiphloi
Calibration Date: 9 April 2024
The Method used: In house method, CAL-WI-58, base on ASTM E 70-07
Traceability: This certificate is traceable to SI Units, Sample Test is assured through primary measurement method Harned cell, through CPAchem Ltd. (ISO/IEC 17034) Certificate No. 938377, 931985, 931984 And pH Scale traceable to the SI Units maintained by National Institute of Metrology (NIMT), Thailand through Industrial Foundation Electrical and Electronics Institute Certificate No. CA20230350EA

Orawan
(Miss Orawan Khlaiphloi)
Person in charge

(Mr. Nitinun Srihawan)
Authorized signatory

This certificate is issued the units of measurement according to the International System of Units (SI). It provides traceability of measurement to international or national standard or other recognized national standard laboratories.
The measurement uncertainty stated is the expanded uncertainty which is obtained from the standard uncertainty multiplied by the coverage factor (k=2) to provide a level of confidence of approximately 95%. It is determined in accordance with the Guide to Expression of Uncertainty in Measurement (GUM).
These results may be affected by deviations from specified conditions. The results relate only to the items tested, calibrated or sampled. The report shall not be reproduced except in full without approval of DKSH Technology Limited.



Certificate No.: C07240167 Page 2 of 3

Calibration Results:

pH Scale

Input	pH Meter Reading			Uncertainty of Measurement (mV)	Coverage Factor (k)
(mV)	(mV)	Error (mV)	(pH)		
414.12	414	-0.12	0.00	0.58	2.00
354.96	355	0.04	1.00	0.58	2.00
295.8	296	0.20	2.00	0.58	2.00
236.64	237	0.36	3.00	0.58	2.00
177.48	178	0.52	4.00	0.58	2.00
118.32	118	-0.32	5.00	0.58	2.00
59.16	59	-0.16	6.00	0.58	2.00
0	0	0.00	7.00	0.58	2.00
-59.16	-59	0.16	8.00	0.58	2.00
-118.32	-118	0.32	9.00	0.58	2.00
-177.48	-177	0.48	10.00	0.58	2.00
-236.64	-236	0.64	11.00	0.58	2.00
-295.8	-296	-0.20	12.00	0.58	2.00
-354.96	-355	-0.04	13.00	0.58	2.00
-414.12	-414	0.12	14.00	0.58	2.00

Practical slope and zero point*

The three-point calibration using three standard buffer solutions; pH 4.008 , pH 6.985 and pH 9.997

-During calibration, display of pH meter reading; pH 4.00 , pH 7.00 and pH 10.01

The practical slope of the pH electrode; 57.01 (mV/pH), 96.37%

The zero point of the pH electrode; 6.88 (pH)

Sample Test Results

Standard Buffer Solution (pH)	Unit Under Calibration (pH)	Difference (pH)	Uncertainty of Measurement (pH)	Coverage Factor (k)
4.008	3.99	-0.018	0.0070	2.00
6.985	7.00	0.015	0.0091	2.00
9.997	10.02	0.023	0.0074	2.00

* Calibration Marked " Not TISI Accredited " in this Certificate have been included for completeness.

The End of Certificate



Certificate of Calibration

Equipment: Digital Thermometer with Probe
Model: SevenEasy pH
Serial No.: 1230525212
Manufacturer: METTLER TOLEDO
ID No.: UAE.WAS.003/2553

Certificate No.: C15240373
Issued Date: 09 April 2024
Job No.: WO-00024208
Page: 1 of 2
Condition: In Condition

Customer: United Analyst and Engineering Consultant Company Limited
3 Soi Udomsuk 41 Sukhumvit Road,
Bangchak, Prakanong, Bangkok 10260 Thailand

Environment Condition: Temperature: 22 °C ± 3 °C
Humidity: 50 %RH ± 20 %RH
Voltage: 220 VAC ± 10 %

Calibration Place: Thermo-Hygro Laboratory, DKSH Technology Limited,
2533 Sukhumvit Road, Bangchak,
Phrakhanong, Bangkok 10260 Thailand

Calibration By: Mr. Nateekarn Mitjit
Calibration Date: 09 April 2024
The Method used: In house method, CAL-WI-19, by comparison with standard thermometer
Traceability: This certificate is traceable to the International System of Unit maintained by Quality Reborn Co.,Ltd. (QR) Certificate No. QR23-1073

(Mr. Nateekarn Mitjit)
Person in charge

(Mr. Pramote Ramrong)
Authorized signatory

This certificate is issued the units of measurement according to the International System of Units (SI). It provides traceability of measurement to international or national standard or other recognized national standard laboratories.
The measurement uncertainty stated is the expanded uncertainty which is obtained from the standard uncertainty multiplied by the coverage factor (k=2) to provide a level of confidence of approximately 95%. It is determined in accordance with the Guide to Expression of Uncertainty in Measurement (GUM).
These results may be affected by deviations from specified conditions. The results relate only to the items tested, calibrated or sampled. The report shall not be reproduced except in full without approval of DKSH Technology Limited.

Certificate No.: C15240373

Page: 2 of 2

Reference standard equipment:

Equipment	Certificate no	Cal. date	Next Cal. date
Digital Thermometer with Probe	QR23-1073	2 May 23	2 May 24

Calibration Results:

Without Adjustment

Sensor Type: RTD

Channel: -

Diameter (mm) 4

Length (mm): 135

Immersion (mm): 110

Calibrate Point (°C)	STD. Reading (°C)	UUC. Reading (°C)	Correction of UUC (°C)	Uncertainty (± °C)
15.0	15.010	15.1	-0.090	0.076
25.0	25.006	25.1	-0.094	0.076
35.0	35.004	35.0	0.004	0.076

The End of Certificate



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL: 0-2717-3000-29 FAX: 0-2719-9484



Cert. No.: 24TM303
Page: 1 of 3

Certificate of Calibration

Equipment : BOD Incubator
Manufacturer : Arco
Model : UIC4-1320
Serial No. : 13URC4S013201
ID No. : UAE.WAO.015/2561
Submitted by : United Analyst and Engineering Consultant Co.,Ltd.
3 Soi Udomsuk 41, Sukhumvit Road,
Bangchak, Phrakhanong,
Bangkok 10260
Location : Lab Floor 2
Received Order : 10 February 2024
Calibration Date : 10 February 2024
Ambient Temperature : (26 ± 10) °C
Relative Humidity : (50 ± 30) %
Calibrated by : Tawatchai Pama
Approved by :
() Pornthippa Tameyakul
(✓) Unnopphol Harachai
() Suwit Imjai
Issue Date : 19 February 2024

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.



Equipment : BOD Incubator
Condition As-Received : Used Item
Reference : 2402-0234OC-1
Result of Calibration :- (*) Without Adjustment
Function of UUC* : Temperature Source
Fresh air setting : Not Available

Cert. No.: 24TM303
Page : 3 of 3

Calibration Point (°C)	UUC* Setting (°C)	UUC* Reading (°C)	Temperature stability (± °C)	Temperature uniformity (°C)	Overall Variation (°C)	Coverage Factor k
20.0	20.1	19.9	0.37	0.72	1.4	2

Calibration Point (°C)	Measured Temperature (°C)									Uncertainty (± °C)
	1	2	3	4	5	6	7	8	9 (ref.)	
20.0	19.873	19.803	20.322	19.690	19.615	19.585	19.612	19.558	19.645	0.58

Average* : The average of 30 values in each position.
Temperature stability : One-half of the greatest maximum difference of measured temperature at any one sensor.
Temperature uniformity : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.
Overall Variation : The Difference of the maximum and minimum measured temperatures throughout observation.
UUC* : Unit Under Calibration
Note : The reported uncertainty of measurement was included stability and excluded uniformity .
The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-oOo-

เอกสารไม่ควบคุม



Equipment : BOD Incubator
Condition As-Received : Used Item
Reference : 2402-0234OC-1
Procedure Used :-
Calibration were conducted using calibration procedure CP-OT02 based on TLAS G-20 according to direct measurement method with Data Acquisition which connected with Resistance Temperature Detector (RTD).
The temperature scale used was based on ITS-90.

Cert. No.: 24TM303
Page : 2 of 3

Condition of this result of calibration

- Reference standard instrument:-

Instrument	Serial No.	Cert. No.	Traceable	Due Date
1) Data Acquisition	MY59003411	23LM208	TPA	27 Dec 2024
- This certificate is valid only to the item calibrated on date and place of calibration.
- This certification is traceable to the International System of Unit.


Remark : TPA : Technology Promotion Association (Thailand - Japan)

Result of Calibration :- (*) Without Adjustment

Function of UUC* : Temperature Source

Fresh air setting : Not Available

Environment during calibration		
	Beginning	Finished
Temp. (°C)	28	31
REL.Humid. (%)	70	65
AC Supply (Volt)	233	234



Probe Installation Details :

a = 10 cm
b = 10 cm
c = 10 cm

Dimension of Chamber :

D = 0.62 m
W = 1.2 m
H = 1.2 m
Capacity = 0.89 m³

Position :	Ref. Std. ID No.:
1	20RTD-2/1
2	20RTD-2/2
3	20RTD-2/3
4	20RTD-2/4
5	20RTD-2/5
6	20RTD-2/6
7	20RTD-2/7
8	20RTD-2/8
9 (ref.)	20RTD-2/9

เอกสารไม่ควบคุม



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3 : EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000 FAX. 0-2719-9484

Cert.No.: 24TW39
Page.: 1 of 2

Certificate of Testing

Equipment : DO Meter
Manufacturer : YSI
Model : 5100
Serial No. : 11B 101863
ID No. : UAE.WAO.004/2554
Received Date : 20 February 2024
Test Date : 21 February 2024
Reference : 2402-0629DSC-1
Submitted by : United Analyst and Engineering Consultant Co.,Ltd.
3 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Laboratory Condition : Temperature (25 ± 5) °C
Humidity (50 ± 20) %
Test Procedure : In - house method : CP-CH9
by Comparison Technique with Azide Modification Method

Tested by : Walalak Sirinthean

Approved by :
Approved Signatory

() Pornthippa Tameyakul
() Unnopphol Harachai
(✓) Saithip Meangmai

Issue Date : 22 February 2024

เอกสารไม่ควบคุม



Cert.No.: 24TW39
Page.: 2 of 2

Condition of this result of calibration

- Reference Standard Instruments :
This certification is traceable to the International System of Unit through the reference standards laboratory of Industrial Calibration Center, Technology Promotion Association (Thailand-Japan).

Instruments	Serial No.	ID No.	Certificate No.	Due Date
1. Burette	-	130BU10	23CG1172	22 Mar 2025
2. Balance	14233821	110RC001	23MM405	16 July 2024

2. Standard Material :-

Material	Manufacturer	Lot.No.	Assay
Sodium Thiosulfate pentahydrate	Merck	AM1763316	100.2%

Result : Dissolved Oxygen Meter Adjustment With Air 100 %
Dissolved Oxygen Probe No.: 22B100125

Titration Method (Azide Modification Method) (mg/L)	DO Meter Reading (mg/L)	Standard Deviation (mg/L)
8.20	8.19	0.0055

This report was certified only for the instrument we tested.It is allowable to use for study Intend to use for advertising and referral purpose is prohibited.This report may not be reproduced other in full,without written approval of the laboratory

-oOo-

เอกสารไม่ควบคุม

Calibration Report

Certificate No.: 2402283-002-01
Equipment: Electronic Balance
Model: XSR2050U
Serial No.: C210683394
Capacity: 220 g
Manufacturer: METTLER TOLEDO
Resolution: 0.00001 g / 0.0001 g
ID No.: UAE.WAO.010/2565

Date of Calibration: 2 April 2024 Page 2 of 4

Environment Condition: Ambient Temperature: 24.5 ± 0.5 °C Relative Humidity: 47.5 ± 2.5 %

Place of Calibration: Laboratory, UNITED ANALYST AND ENGINEERING CONSULTANT CO., LTD.

Condition of Equipment: Good Condition

Condition of This Results of Calibration:

1. Calibration Method: NFI Method W-MA-001 In-House Method based on UKAS Lab 14 : 2019

2. Reference Standards:

Reference Standard	Model	Serial No.	Calibrated By	Certificate No.	Due Date
Standard Weight Class E2	1mg to 200g	8505567572	TCS	M23040535	8 April 2024
Instrument	Model	Serial No.	Calibrated By	Certificate No.	Due Date
Thermo-Hygro Meter	608-H1	NFLBTH 015/23	Quality Reborn	QB24-0343	9 February 2025

3. This certification is traceable to SI UNIT

4. This certificate was certified only for the instrument we calibrated.

5. This result of calibration was found accurate as shown on date and place of calibration only.

Calibration Results:


1. Repeatability of Reading:

Nominal Value (g)	Standard Deviation of Reading (g)
40	0.000042
80	0.000052
100	0.000048
200	0.000048

2. Off-Center Error:

A mass of 100 g was placed and moved to various position on pan.

The balance reading obtained is given in the table.



1	2	3	4	5	6	(Maximum Difference)
(g)	(g)	(g)	(g)	(g)	(g)	(g)
100.0000	100.0001	99.9999	99.9999	100.0001	100.0000	0.0001

F-CS-012 Revision: 01 Date: 20-04-65

2008 ๒๕๕๑ ถนนสุขุมวิท 35 แขวงคลองเตย เขตวัฒนา กรุงเทพมหานคร 10110 ประเทศไทย
2008 Soi 35, Asoin Amarin Road, Bang Yi Khan Subdistrict, Bang Phai District, Bangkok 10110, Thailand
Tel : +66(0) 2422 8668 Fax : +66(0) 2422 8545



Calibration Report

Certificate No.: 2402283-002-01
Equipment: Electronic Balance
Model: XSR2050U
Serial No.: C210683394
Capacity: 220 g
Manufacturer: METTLER TOLEDO
Resolution: 0.00001 g / 0.0001 g
ID No.: UAE.WAO.010/2565

Date of Calibration: 2 April 2024 Page 3 of 4

Calibration Results: (Continued)

Calibration Range: 0 - 80 g

Calibration Adjustment: Internal Calibration

3. Departure from Nominal Value: (Range: 0 - 80 g ; Resolution: 0.00001 g)

Nominal Value (g)	Standard Value (g)	Average Reading (g)	Correction (g)	Uncertainty (± g)	Coverage Factor
Unload	0.000000	0.00000	0.00000	0.0000086	2.00
0.001	0.001003	0.00101	-0.00001	0.0000089	2.00
0.005	0.005003	0.00500	0.00000	0.0000092	2.00
0.01	0.010003	0.01000	0.00000	0.0000089	2.00
0.05	0.049996	0.05000	0.00000	0.0000096	2.00
0.1	0.100011	0.10000	0.00001	0.000011	2.00
0.5	0.500016	0.50001	0.00001	0.000014	2.00
1	1.000003	1.00002	-0.00002	0.000016	2.00
2	2.000023	2.00001	0.00001	0.000017	2.00
5	5.000017	5.00002	0.00000	0.000020	2.00
10	10.000009	10.00000	0.00001	0.000026	2.00
20	20.000031	20.00000	0.00003	0.000037	2.00
30	30.000040	30.00001	0.00003	0.000050	2.00
50	50.000028	50.00002	0.00001	0.000068	2.00
80	80.000068	80.00002	0.00005	0.00011	2.00

F-CS-012 Revision: 01 Date: 20-04-65

2008 ๒๕๕๑ ถนนสุขุมวิท 35 แขวงคลองเตย เขตวัฒนา กรุงเทพมหานคร 10110 ประเทศไทย
2008 Soi 35, Asoin Amarin Road, Bang Yi Khan Subdistrict, Bang Phai District, Bangkok 10110, Thailand
Tel : +66(0) 2422 8668 Fax : +66(0) 2422 8545



Calibration Report

Certificate No.: 2402283-002-01
Equipment: Electronic Balance
Model: XSR2050U
Serial No.: C210683394
Capacity: 220 g
Manufacturer: METTLER TOLEDO
Resolution: 0.00001 g / 0.0001 g
ID No.: UAE.WAO.010/2565

Date of Calibration: 2 April 2024 Page 4 of 4

Calibration Results: (Continued)

Calibration Range: 81 - 200 g

Calibration Adjustment: Internal Calibration

3. Departure from Nominal Value: (Range: 81 - 200 g ; Resolution: 0.0001 g)

Nominal Value (g)	Standard Value (g)	Average Reading (g)	Correction (g)	Uncertainty (± g)	Coverage Factor
90	90.00010	90.0001	0.0000	0.00015	2.00
100	100.00006	100.0001	0.0000	0.00015	2.00
110	110.00007	110.0001	0.0000	0.00016	2.00
120	120.00009	120.0000	0.0001	0.00017	2.00
130	130.00010	130.0000	0.0001	0.00019	2.00
140	140.00014	140.0000	0.0001	0.00020	2.00
150	150.00009	150.0001	0.0000	0.00020	2.00
160	160.00010	160.0001	0.0000	0.00022	2.00
170	170.00012	170.0001	0.0000	0.00023	2.00
200	200.00016	200.0002	0.0000	0.00028	2.00

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k, providing a level of confidence of approximately 95 %.

F-CS-012 Revision: 01 Date: 20-04-65

2008 ๒๕๕๑ ถนนสุขุมวิท 35 แขวงคลองเตย เขตวัฒนา กรุงเทพมหานคร 10110 ประเทศไทย
2008 Soi 35, Asoin Amarin Road, Bang Yi Khan Subdistrict, Bang Phai District, Bangkok 10110, Thailand
Tel : +66(0) 2422 8668 Fax : +66(0) 2422 8545

Calibration Certificate

Certificate No.: 2500116-001-01
Client name: UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.
Address: 3 Soi Udomsuk 41, Sukhumvit Road, Bangchack, Prakhonong, Bangkok 10260

Equipment: CHAMBER (Hot Air Oven)

Manufacturer: MEMMERT

Model: UF55

Serial No.: B216.1666

ID No.: UAE.WAO.027/2559

Order No.: 2500116

Operation No.: 2500116-001

Date of Receipt: 8 October 2024

Date of Calibration: 8 October 2024

Calibrated by Mr.Yothin Charoensuk
Scientist

Approved by (Mr.Pheraphat Tuanjit)
Manager, Division of Calibration Laboratory
Responsible for the Technical Management Team

Date of Issue: 15 October 2024

The uncertainties are for a confidence probability of approximately 95 %.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the National Food Institute.

F-CS-009 Revision: 01 Date: 20-04-65

2008 ๒๕๕๑ ถนนสุขุมวิท 35 แขวงคลองเตย เขตวัฒนา กรุงเทพมหานคร 10110 ประเทศไทย
2008 Soi 35, Asoin Amarin Road, Bang Yi Khan Subdistrict, Bang Phai District, Bangkok 10110, Thailand
Tel : +66(0) 2422 8668 Fax : +66(0) 2422 8545

Calibration Report

Certificate No.: 2500116-001-01
Equipment: CHAMBER (Hot Air Oven)
Model: UF55 Serial No.: B216.1666
Resolution: 0.1 °C ID No.: UAE.WAO.027/2559
Manufacturer: MEMMERT
Date of Calibration: 8 October 2024 Page 2 of 3

Location: Laboratory, UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.
Environment Condition:
Ambient Temperature (30.3 ± 1) °C
Relative Humidity (55 ± 1) %
Line Voltage (230 ± 3) Volt

Condition of this results of Calibration:

- This instrument was calibrated by insert 9 standard thermometer into its chamber and calibration according to W-TE-014 Based on TLAS G-20-1/02-08 (E): Guidelines for Calibration and Checks of Temperature Controlled Enclosures.
- The temperature scale used was based on ITS - 90.
- All data show below were final values and the initial data may be obtained upon request.

2. Reference Standard Instrument :

Instrument	Model	Serial No./ID No.	Certificate No.	Due Date	Through
Digital Thermometer with sensor	34972A	MYS7003188	TE 670486-01	8 June 2025	NATIONAL FOOD INSTITUTE
	RTD	CHP201-209/RTD#201-209			

- This certificate is traceable to International System of Units (SI Units).
- This certificate was certified only for the instrument we calibrated.
- This result of calibration was found accurate as shown on date and place of calibration only.
- Condition of Calibrated item : Good

UUC Description :

Time of Record 1 Hour 9 Minute At 104.0, 140.0 and 180.0 °C
Fresh air Damper - Open Position -
X Close Fan 40%
- Not Available

- Result of Calibration : X Without adjustment After adjustment

F-CS-012 Revision: 01 Date: 20-04-65

เอกสารไม่ควบคุม



Calibration Report

Certificate No.: 2500116-001-01
Equipment: CHAMBER (Hot Air Oven)
Model: UF55 Serial No.: B216.1666
Resolution: 0.1 °C ID No.: UAE.WAO.027/2559
Manufacturer: MEMMERT
Date of Calibration: 8 October 2024 Page 3 of 3

Calibration point: 104.0, 140.0 and 180.0 °C

Calibration result:

Calibration Condition	Temperature (°C)	Relative Humidity (%)	Line Voltage (Volt)
MIN	29.3	54	227.0
MAX	31.2	56	232.0




Table 1 : Reporting of Temperature

Calibration point (°C)	Measured Temperature (°C) @ Sensor No. (Sensor No.9 is REF)									Uncertainty ± (°C)
	# 1	# 2	# 3	# 4	# 5	# 6	# 7	# 8	# 9	
104.0	103.89	103.66	103.88	103.89	104.40	103.98	103.70	104.10	104.15	0.53
140.0	139.85	139.53	139.67	139.88	140.67	140.00	139.60	140.25	140.23	0.73
180.0	179.63	179.22	179.71	179.76	181.03	180.06	179.41	180.87	180.39	0.90

Table 2 : Reporting of Characterization Result

UUC* Setting (°C)	UUC* Reading (°C)			Stability ± (°C)	Uniformity (°C)	Overall Variation (°C)
	MIN	MAX	Average			
104.0	104.0	104.0	104.0	0.15	0.49	0.88
140.0	140.0	140.0	140.0	0.13	0.71	1.2
180.0	180.0	180.0	180.0	0.13	1.2	1.9

Note The quoted uncertainty include " Stability " and " Loading effect (20% of Temp Uniformity) "

UUC* = Unit Under Calibration

Stability = One-half of the greatest maximum difference of measured temperatures at any one sensors, for at least half an hour after reaching steady state.

Uniformity = The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time.

Overall Variation = The difference of the maximum and minimum measured temperatures throughout observation time.

The report uncertainty of measurement was based on standard uncertainty multiplied by coverage factor k= 2, providing a level of confidence of approximately 95 %.

----- End -----

F-CS-012 Revision: 01 Date: 20-04-65

เอกสารไม่ควบคุม



Certificate No.: HIT-2417-0568

Page : 1 of 2

CERTIFICATE OF CALIBRATION

Equipment : COD Test Tube Heater
Meter Model : HI839800-02 Serial No. : 1147807
Tube Heater : 25 Vial Capacity Resolution : 0.1°C
Temperature Range : (-10 to 160)°C Temperature of Reaction : 150°C
Manufacturer : Hanna Instruments Made in : Romania
Condition As-Received : Used Product Reference : RE240681
Ambient Temperature : (25 ± 2)°C Relative Humidity : (50 ± 15)%RH

Customer name : United Analyst and Engineering Consultant Co., Ltd.
3 Soi Udomsuk 41, Sukhumvit Rd., Bangehak,
Phrakhanong, Bangkok 10260

Received date : 22 April 2024

Calibrate date : 23 April 2024

Issue date : 25 April 2024

Calibrated Location : Hanna Instruments (Thailand) Ltd.

Calibration Procedure : This calibrator was conducted by using in-house: calibration procedure
CP-04 by using certified reference standard instruments.

Calibrated by : Mr. Pichit Petthong

Mr. Channarong Soinak

Approved by :

Mr. Anan Suwanchaisakul

Authorized Signatory



This certificate was certified only for the instrument we calibrated.

This result of calibration was found accurate on date and place of calibration only.

** This certificate may not be reproduced other than in full, except with the prior written **

approval of the head of Hanna Instrument (Thailand).

เอกสารไม่ควบคุม

Certificate No.: HIT-2417-0568

Page : 2 of 2

Condition of this calibration result:

Reference Standard Instruments : This certification is traceable to the international unit of unit maintained through:

Instruments	Model	Serial No.	Certificate No.	Traceable
Data Acquisition Switch Unit	34970A	MY44065265	WK2307-164-I	WK Electric Co., Ltd.
Digital Thermo-Hygrometer	HT-771SD	AI.07155	24H41	Technology Promotion Association (Thailand-Japan).

Calibration Result:

Measurement Temperature Source Accuracy for COD Reactor.

Capacity (Vial)	Nominal Value (°C)	Average Value (°C)	Uncertainty of Measurement (±°C)
25 Vial	150.0	149.8	0.49

Unit : °C

(1A)	(2A)	(3A)	(4A)	(5A)
148.901	149.249	149.950	150.042	149.186
(1B)	(2B)	(3B)	(4B)	(5B)
149.724	149.578	149.852	150.100	150.117
(1C)	(2C)	(3C)	(4C)	(5C)
149.863	149.799	150.233	149.847	149.977
(1D)	(2D)	(3D)	(4D)	(5D)
149.550	149.666	149.958	149.744	149.819
(1E)	(2E)	(3E)	(4E)	(5E)
150.044	149.869	149.361	149.973	149.654

Figure: Shows the location of the temperature source.

The report uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k= 2, providing a level of confidence of approximately 95%

** End of certificate **

เอกสารไม่ควบคุม

Verification Certificate

Substitute for Certificate No.: 2402957-001-01
Certificate No.: 2402957-001-02
Client name: UNITED ANALYST AND ENGINEERING CONSULTANT CO., LTD.
Address: 3 Soi Udomsuk 41, Sukhumvit Road, Bangchack, Prakhnong, Bangkok 10260

Page 1 of 4


Equipment: HEATING BLOCK DIGESTION
Manufacturer: FOSS
Model: 2520
Serial No.: 91794469
ID No.: UAE.WAS.011/2560
Order No.: 2402957
Operation No.: 2402957-001
Date of Receipt: 23 May 2024
Date of Calibration: 23-24 May 2024

Calibrated by Mr.Jerawut Prapawuttipong Scientist
Approved by (Mr.Pheraphat Tuanjit) Manager, Division of Calibration Laboratory
Date of Issue: 18 June 2024

The uncertainties are for a confidence probability of approximately 95 %.
This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory.

F-CS-011 Revision: 01 Date: 20-04-65

2008 ซอย 35 ถนนอนุراج แขวงบางพลัด เขตบางพลัด กรุงเทพมหานคร 10700
2008 Soi 35, Anuraj Road, Bang Yai Khan Subdistrict, Bang Phai District, Bangkok 10700, Thailand
Tel : +66(0) 2442 8548 Fax : +66(0) 2442 8545



Verification Report

Certificate No.: 2402957-001-02
Equipment: HEATING BLOCK DIGESTION
Model: 2520 Serial No.: 91794469
Resolution: 1 °C ID No.: UAE.WAS.011/2560
Manufacturer: FOSS
Date of Calibration: 23-24 May 2024

Page 2 of 4

Location: UNITED ANALYST AND ENGINEERING CONSULTANT CO., LTD.
Environment Condition: Ambient Temperature (25 ± 3) °C
Relative Humidity (55 ± 15) %
Line Voltage (220 ± 10) Volt

- Condition of this results of Calibration:
1. This instrument was calibrated by insert standard thermocouples type R into its heating block digestion and compared to temperature obtained from reference standards thermometer at calibrated point.
- The temperature scale used was based on ITS - 90 .
- All data show below were final values and the initial data may be obtained upon request.
2. Reference Standard Instrument :

Table with 5 columns: Instrument, Model, Serial No., Certificate No., Due Date, Through. It lists a Digital Thermometer with Thermocouple, Type R, TCF 101-103 / DTF 101-103, TC23/0048, 2-Jun-2024, and N.M. Technical Center Laboratory.

- 3. This certificate is traceable to international system of units (SI Units).
4. This certificate was certified only for the instrument we calibrated.
5. This result of calibration was found accurate as shown on date and place of calibration only.
6. Condition of Calibrated item : Good
UUC* Description
Time of Record Hour 30 Minute At 380 °C
7. Result of Calibration : [X] Without adjustment [] After adjustment

F-CS-012 Revision: 01 Date: 20-04-65

2008 ซอย 35 ถนนอนุراج แขวงบางพลัด เขตบางพลัด กรุงเทพมหานคร 10700
2008 Soi 35, Anuraj Road, Bang Yai Khan Subdistrict, Bang Phai District, Bangkok 10700, Thailand
Tel : +66(0) 2442 8548 Fax : +66(0) 2442 8545



Verification Report

Certificate No.: 2402957-001-02
Equipment: HEATING BLOCK DIGESTION
Model: 2520 Serial No.: 91794469
Resolution: 1 °C ID No.: UAE.WAS.011/2560
Manufacturer: FOSS
Date of Calibration: 23-24 May 2024
Calibration point: 380 °C
Calibration result: Reporting of Temperature

Page 3 of 4

Table with 6 columns: Block No., UUC* Setting (°C), UUC* Reading (°C), Stability (±°C), Standard Thermometer (°C), Uncertainty (±°C). It contains 20 rows of calibration data for a heating block digestion at 380 °C.

Note:
- UUC* = Unit Under Calibration
- Immersion depth of standard thermometer in tube level high of sand is equal heater plate of UUC.
- Stability = One-half of the greatest maximum difference of measured temperatures at one sensors, for at least half an hour after reaching steady state.

F-CS-012 Revision: 01 Date: 20-04-65

2008 ซอย 35 ถนนอนุراج แขวงบางพลัด เขตบางพลัด กรุงเทพมหานคร 10700
2008 Soi 35, Anuraj Road, Bang Yai Khan Subdistrict, Bang Phai District, Bangkok 10700, Thailand
Tel : +66(0) 2442 8548 Fax : +66(0) 2442 8545




Verification Report

Certificate No.: 2402957-001-02
Equipment: HEATING BLOCK DIGESTION
Model: 2520 Serial No.: 91794469
Resolution: 1 °C ID No.: UAE.WAS.011/2560
Manufacturer: FOSS
Date of Calibration: 23-24 May 2024
Calibration point: 380 °C
Calibration result: Continued

Page 4 of 4

Figure 1. Location of Reference Standard and Block Diagram of Digestion Unit

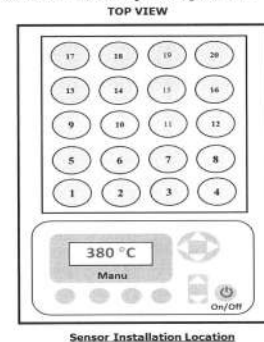

Remark: Edited Date of Calibration from 23-24 May 204 to 23-24 May 2024.

Note:
- UUC* = Unit Under Calibration
- Immersion depth of standard thermometer in tube level high of sand is equal heater plate of UUC.
- Stability = One-half of the greatest maximum difference of measured temperatures at one sensors, for at least half an hour after reaching steady state.

The report uncertainty of measurement was based on standard uncertainty multiplied by coverage factor k= 2, providing a level of confidence of approximately 95 %.

***** End *****

F-CS-012 Revision: 01 Date: 20-04-65

2008 ซอย 35 ถนนอนุراج แขวงบางพลัด เขตบางพลัด กรุงเทพมหานคร 10700
2008 Soi 35, Anuraj Road, Bang Yai Khan Subdistrict, Bang Phai District, Bangkok 10700, Thailand
Tel : +66(0) 2442 8548 Fax : +66(0) 2442 8545



FOSS

Customer Service Report

Date:	9 Feb 2024	Report No:	9810
Customer:	UAE	Address:	BANGKOK
Instrument:	KJ200	Serial:	91790524
Hours	Travel To Customer	Labour	Travel From Customer
Start	08:30	09:30	14:30
Finish	09:30	12:00	16:30

Job Type					
Application	Special	Standard			
Normal	Courtesy Visit	Installation	Quote	Training	
Distributor	PMA Onboarding	Quote	In House		
Internal	Warranty	Repair	PM		
Digital Service	Sales Support	Remote	Other		

PO/Quote Number: If applicable

PMA Type: FOSSC C If applicable Contract No. If applicable

Details of Work / Test	Condition / Status
# PM KJ200	
- ตรวจสอบเครื่องวัดค่า PM	
- ตรวจสอบค่า 3 วัน 100 m	
- Airline 50 m - 20 m	
- ตรวจสอบค่า PM kit	
- ตรวจสอบค่า 3 วัน	
# ตรวจสอบ SOPH Mead - ตรวจสอบเครื่องวัดค่า PM	
10000725 Serial New Complete IPC	
Instrument Ready for Use	OK / Not OK If not OK - Comment

Part No.	Batch	Description	Qty
10099965	14.12.2020	FOSS PM kit lot 300 lot 101 Annalysse 8100	1

I confirm this report is accurate and complete	
Signed FOSS	Signed Customer
Name	Name
Would you be willing to participate in a brief survey in order to tell us how we performed?	
Email	

เอกสารไม่ควบคุม



Request No. 25-67 / 0275

MTC. ACL.No. 358 / 67

CALIBRATION CERTIFICATE

NOMENCLATURE : 1. Atomic Absorption Spectrophotometer "Agilent Technologies"

Model AA240FS, Serial No. MY13160001

2. Working standard solution "Inorganic Ventures"

Multi Analyte Custom Grade Solution, Lot No. S2-ME675610

SUBMITTED BY : United Analyst and Engineering Consultant Co., Ltd.

3 Sol Udornskul 41, Sukhumvit Road, Bangchak, Prakanong, Bangkok 10260

CALIBRATION PROCEDURE : 1. Performance Verification of Atomic Absorption Spectrophotometer (WI-500-02-30)

2. Estimation Uncertainty of Measurement in Analytical Chemistry (QP-513)

CALIBRATION RANGE: 0.02, 0.10, 0.30, 0.50, 0.70 mg/l at 228.8 nm.Cd, 0.10, 0.20, 0.30, 0.50, 0.70 mg/l at 357.9 nm.Cr, 0.05, 0.10, 0.30, 0.50, 0.70 mg/l at 324.7 nm.Cu, 0.10, 0.30, 0.50, 0.70, 1.00 mg/l at 248.3 nm.Fe, 0.20, 0.50, 0.70, 1.00, 1.50 mg/l at 217.0 nm.Pb, 0.05, 0.10, 0.30, 0.50, 0.70 mg/l at 279.5 nm.Mn, 0.10, 0.30, 0.50, 0.70, 1.00 mg/l at 232.0 nm.Ni, 0.05, 0.10, 0.30, 0.50, 0.70 mg/l at 213.9 nm.Zn

CALIBRATION DATE : 2 February 2024

REFERENCE MATERIAL : Traceable to NIST "Agilent Technologies", "CARLO ERBA"

Cadmium Lot No. 0006589926, Chromium Lot No. 0112384886, Copper Batch No. T117098A, Iron Batch No. T126087A, Lead Lot No. 1227873, Manganese Batch No. T109228A, Nickel Batch No. T270178A, Zinc Batch No. T820140A

AMBIENT CONDITIONS : Temperature 25 ± 5 °C Relative humidity 50 ± 20 %

The Atomic Absorption Spectrophotometer has been calibrated against Reference Material traceable to National Institute of Standards and Technology (NIST) by The Analytical Chemistry Laboratory. The results are attached herewith.

Calibrated by	Atipat	Approved by	Suladda
	(Mr. Atipat Ratana)		(Miss Suladda Deawong)
			Director of Analytical Chemistry Laboratory
			Ref. 2015267020100454001
			Issued Date : 11 March 2024

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FMBL.MTC.002 Rev.4

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9000
Fax. (66) 0 2577 9009
E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

Office/Laboratory
Sol IC, Bangpoo Industrial Estate, Sukhumvit Road,
Amphoe Muang Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
Fax. (66) 0 2323 9165
E-mail : mtg@tistr.or.th

Office
196 Phahonyothin Road, Chatuchak, Bangkok 10900,
Thailand
Tel. (66) 0 2577 9000
Fax. (66) 0 2577 9009
E-mail : sumalee@tistr.or.th

เอกสารไม่ควบคุม

FOSS

Customer Service Report

Date:	9 Feb 2024	Report No:	9810
Customer:	UAE	Address:	BANGKOK
Instrument:	KJ200	Serial:	91790524
Hours	Travel To Customer	Labour	Travel From Customer
Start	08:30	09:30	14:30
Finish	09:30	12:00	16:30

Job Type					
Application	Special	Standard			
Normal	Courtesy Visit	Installation	Quote	Training	
Distributor	PMA Onboarding	Quote	In House		
Internal	Warranty	Repair	PM		
Digital Service	Sales Support	Remote	Other		

PO/Quote Number: If applicable

PMA Type: FOSSC C If applicable Contract No. If applicable

Details of Work / Test	Condition / Status
# PM KJ200	
- ตรวจสอบเครื่องวัดค่า PM	
- ตรวจสอบค่า 3 วัน 100 m	
- Airline 50 m - 20 m	
- ตรวจสอบค่า PM kit	
- ตรวจสอบค่า 3 วัน	
# ตรวจสอบ SOPH Mead - ตรวจสอบเครื่องวัดค่า PM	
10000725 Serial New Complete IPC	
Instrument Ready for Use	OK / Not OK If not OK - Comment

Part No.	Batch	Description	Qty
10099965	14.12.2020	FOSS PM kit lot 300 lot 101 Annalysse 8100	1

I confirm this report is accurate and complete	
Signed FOSS	Signed Customer
Name	Name
Would you be willing to participate in a brief survey in order to tell us how we performed?	
Email	

เอกสารไม่ควบคุม



Request No. 25-67 / 0275

1 / 5

MTC. ACL. No. 358 / 67

CALIBRATION DATA

1. Noise Level

Element	Cd	Cr	Cu	Fe	Pb	Mn	Ni	Zn
Absorbance	0.0006	0.0004	-0.0003	0.0001	-0.0011	-0.0005	0.0008	0.0004
	0.001	0.0017	-0.0009	0.0008	0.0001	0.0002	-0.0003	0.0007
	0.0006	0.0017	-0.0020	0.0005	0.0005	0.0004	0.0013	0.0014
	0.0001	0.0018	-0.0007	0.0005	0.0004	-0.0003	-0.0001	0.0010
	-0.0001	0.0019	-0.0014	0.0003	0.0010	0.0000	0.0002	-0.0001
	0.0011	0.0014	-0.0017	0.0009	-0.0008	0.0004	0.0006	0.0010
	-0.0002	0.0015	-0.0015	0.0003	0.0002	-0.0008	0.0009	0.0013
	0.0006	0.0012	-0.0001	0.0006	0.0008	0.0001	-0.0002	0.0013
	0.0008	0.0009	-0.0003	0.0003	0.0005	0.0002	0.0001	0.0007
	0.0012	0.0011	-0.0012	0.0008	0.0003	0.0004	0.0004	0.0013
	0.0003	0.0015	-0.0019	0.0001	-0.0002	0.0000	-0.0003	0.0003
	0.0005	0.0017	-0.0019	-0.0007	0.0000	-0.0007	0.0005	0.0005
	-0.0006	0.0016	0.0000	0.0006	-0.0001	0.0013	0.0006	0.0010
	0.0003	0.0011	-0.0002	0.0001	-0.0007	0.0009	0.0009	0.0002
	0.0003	0.0012	-0.0011	0.0007	-0.0003	-0.0003	0.0010	0.0009
	0.0004	0.0018	-0.0016	-0.0004	-0.0006	0.0008	0.0007	0.0007
	-0.0001	0.0018	-0.0018	0.0013	-0.0006	-0.0001	0.0014	0.0006
	0.0003	0.0017	-0.0001	0.0001	-0.0012	-0.0004	0.0001	0.0002
	0.0010	0.0018	-0.0007	0.0003	-0.0005	-0.0002	0.0001	0.0003
	0.0004	0.0019	-0.0008	-0.0001	-0.0004	0.0003	0.0002	0.0008
Average Absorbance	0.000	0.001	-0.001	0.000	0.000	0.000	0.000	0.001

Continue 2 / 5

INDUSTRIAL METROLOGY AND TESTING SERVICE CENTRE

The results relate only to the items tested/calibrated or value assigned.
Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FMBL.MTC.002 Rev.4

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9000
Fax. (66) 0 2577 9009
E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

Office/Laboratory
Sol IC, Bangpoo Industrial Estate, Sukhumvit Road,
Amphoe Muang Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
Fax. (66) 0 2323 9165
E-mail : mtg@tistr.or.th

Office
196 Phahonyothin Road, Chatuchak, Bangkok 10900,
Thailand
Tel. (66) 0 2577 9000
Fax. (66) 0 2577 9009
E-mail : sumalee@tistr.or.th

เอกสารไม่ควบคุม



Request No. 25-67 / 0275

2 / 5

MTC. ACL. No. 358 / 67

2. Precision

Element	Conc. (mg/l)	Absorbance										Ave. Abs.	SD	%RSD
Cd	0.02	0.0078	0.0076	0.0069	0.0075	0.0071	0.0070	0.0076	0.0074	0.0077	0.0067	0.007	0.0004	5.15
	0.30	0.1008	0.1007	0.0999	0.0997	0.1000	0.0996	0.1008	0.1002	0.1005	0.0999	0.100	0.0005	0.46
	0.70	0.2301	0.2306	0.2277	0.2305	0.2310	0.2295	0.2290	0.2293	0.2305	0.2296	0.230	0.0010	0.42
Cr	0.10	0.0094	0.0093	0.0093	0.0098	0.0094	0.0095	0.0090	0.0090	0.0094	0.0090	0.009	0.0003	2.75
	0.30	0.0241	0.0236	0.0221	0.0238	0.0231	0.0226	0.0231	0.0223	0.0230	0.0231	0.023	0.0006	2.75
	0.70	0.0500	0.0500	0.0500	0.0524	0.0499	0.0511	0.0509	0.0512	0.0515	0.0504	0.051	0.0008	1.63
Cu	0.05	0.0061	0.0062	0.0064	0.0061	0.0069	0.0069	0.0061	0.0062	0.0064	0.0061	0.006	0.0003	5.00
	0.30	0.0419	0.0411	0.0402	0.0407	0.0405	0.0404	0.0399	0.0400	0.0399	0.0400	0.040	0.0006	1.58
	0.70	0.0960	0.0960	0.0960	0.0959	0.0947	0.0955	0.0952	0.0951	0.0955	0.0956	0.096	0.0005	0.48
Fe	0.10	0.0096	0.0101	0.0103	0.0100	0.0099	0.0096	0.0106	0.0099	0.0105	0.0102	0.010	0.0003	3.38
	0.50	0.0424	0.0415	0.0428	0.0427	0.0421	0.0426	0.0413	0.0430	0.0421	0.0419	0.042	0.0006	1.33
	1.00	0.0830	0.0839	0.0847	0.0834	0.0832	0.0820	0.0839	0.0838	0.0837	0.0845	0.084	0.0008	0.92
Pb	0.20	0.0078	0.0074	0.0078	0.0078	0.0076	0.0078	0.0077	0.0078	0.0078	0.0077	0.008	0.0001	1.71
	0.70	0.0278	0.0273	0.0271	0.0267	0.0270	0.0264	0.0274	0.0273	0.0269	0.0269	0.027	0.0004	1.45
	1.50	0.0551	0.0548	0.0552	0.0555	0.0547	0.0546	0.0544	0.0544	0.0549	0.0547	0.055	0.0004	0.64
Mn	0.05	0.0116	0.0107	0.0110	0.0103	0.0108	0.0108	0.0112	0.0107	0.0109	0.0108	0.011	0.0003	3.15
	0.30	0.0650	0.0649	0.0649	0.0651	0.0646	0.0646	0.0649	0.0646	0.0640	0.0648	0.065	0.0003	0.48
	0.70	0.1463	0.1465	0.1459	0.1471	0.1475	0.1474	0.1487	0.1473	0.1462	0.1468	0.147	0.0008	0.56
Ni	0.10	0.0095	0.0100	0.0096	0.0103	0.0102	0.0096	0.0100	0.0095	0.0097	0.0096	0.010	0.0003	3.04
	0.50	0.0443	0.0433	0.0438	0.0444	0.0430	0.0437	0.0444	0.0437	0.0438	0.0434	0.044	0.0005	1.09
	1.00	0.0812	0.0820	0.0834	0.0829	0.0818	0.0829	0.0831	0.0835	0.0816	0.0819	0.082	0.0008	0.99
Zn	0.05	0.0374	0.0377	0.0373	0.0377	0.0374	0.0377	0.0373	0.0371	0.0371	0.0374	0.037	0.0002	0.61
	0.30	0.1985	0.1993	0.1975	0.1992	0.1979	0.1988	0.1995	0.1985	0.1974	0.2004	0.199	0.0009	0.47
	0.70	0.4027	0.4031	0.4019	0.4021	0.4023	0.3981	0.4042	0.4025	0.3993	0.3997	0.402	0.0019	0.48

Continue 3 / 5

INDUSTRIAL METROLOGY AND TESTING SERVICE CENTRE

The results relate only to the items tested/calibrated or value assigned.
Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BLMTC.002 Rev.4

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9000
Fax. (66) 0 2577 9009
E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

Office/Laboratory
Soi 1/C, Bangpoo Industrial Estate, Sukhumvit Road,
Amphoe Muang, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
Fax. (66) 0 2323 9165
E-mail : mtg@tistr.or.th

Office
196 Phahonyothin Road, Chatuchak, Bangkok 10900,
Thailand
Tel. (66) 0 2577 9000
Fax. (66) 0 2577 9009
E-mail : sumalee@tistr.or.th

เอกสารไม่ควบคุม



Request No. 25-67 / 0275

4 / 5

MTC. ACL. No. 358 / 67

3.4 Reading on wavelength- Iron (Fe) at 248.3 nm.

Element	Standard Value of RM (mg/l)	Reading (mg/l)	Error of Measurement (mg/l)	Error of Measurement (%)	Uncertainty (mg/l)
Fe	0.100	0.104	0.005	4.60	± 0.014
	0.500	0.482	-0.018	3.55	± 0.016
	1.006	0.968	-0.038	3.75	± 0.029

3.5 Reading on wavelength- Lead (Pb) at 217.0 nm.

Element	Standard Value of RM (mg/l)	Reading (mg/l)	Error of Measurement (mg/l)	Error of Measurement (%)	Uncertainty (mg/l)
Pb	0.201	0.202	0.001	0.34	± 0.014
	0.706	0.719	0.012	1.73	± 0.030
	1.513	1.459	-0.054	3.57	± 0.061

3.6 Reading on wavelength- Manganese (Mn) at 279.5 nm.

Element	Standard Value of RM (mg/l)	Reading (mg/l)	Error of Measurement (mg/l)	Error of Measurement (%)	Uncertainty (mg/l)
Mn	0.0505	0.050	0.000	0.83	± 0.005
	0.3031	0.306	0.003	1.12	± 0.007
	0.7023	0.698	-0.004	0.62	± 0.014

Continue 5 / 5

INDUSTRIAL METROLOGY AND TESTING SERVICE CENTRE

The results relate only to the items tested/calibrated or value assigned.
Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BLMTC.002 Rev.4

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9000
Fax. (66) 0 2577 9009
E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

Office/Laboratory
Soi 1/C, Bangpoo Industrial Estate, Sukhumvit Road,
Amphoe Muang, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
Fax. (66) 0 2323 9165
E-mail : mtg@tistr.or.th

Office
196 Phahonyothin Road, Chatuchak, Bangkok 10900,
Thailand
Tel. (66) 0 2577 9000
Fax. (66) 0 2577 9009
E-mail : sumalee@tistr.or.th

เอกสารไม่ควบคุม



Request No. 25-67 / 0275

3 / 5

MTC. ACL. No. 358 / 67

3. Trueness

3.1 Reading on wavelength- Cadmium (Cd) at 228.8 nm.

Element	Standard Value of RM (mg/l)	Reading (mg/l)	Error of Measurement (mg/l)	Error of Measurement (%)	Uncertainty (mg/l)
Cd	0.020	0.020	0.000	1.10	± 0.005
	0.301	0.301	0.000	0.11	± 0.005
	0.707	0.693	-0.013	1.85	± 0.008

3.2 Reading on wavelength- Chromium (Cr) at 357.9 nm.

Element	Standard Value of RM (mg/l)	Reading (mg/l)	Error of Measurement (mg/l)	Error of Measurement (%)	Uncertainty (mg/l)
Cr	0.1007	0.104	0.004	3.49	± 0.009
	0.3035	0.297	-0.006	2.11	± 0.012
	0.7071	0.685	-0.023	3.19	± 0.023

3.3 Reading on wavelength- Copper (Cu) at 324.7 nm.

Element	Standard Value of RM (mg/l)	Reading (mg/l)	Error of Measurement (mg/l)	Error of Measurement (%)	Uncertainty (mg/l)
Cu	0.051	0.047	-0.004	7.58	± 0.003
	0.303	0.296	-0.007	2.19	± 0.009
	0.704	0.698	-0.005	0.74	± 0.020

Continue 4 / 5

INDUSTRIAL METROLOGY AND TESTING SERVICE CENTRE

The results relate only to the items tested/calibrated or value assigned.
Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BLMTC.002 Rev.4

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9000
Fax. (66) 0 2577 9009
E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

Office/Laboratory
Soi 1/C, Bangpoo Industrial Estate, Sukhumvit Road,
Amphoe Muang, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
Fax. (66) 0 2323 9165
E-mail : mtg@tistr.or.th

Office
196 Phahonyothin Road, Chatuchak, Bangkok 10900,
Thailand
Tel. (66) 0 2577 9000
Fax. (66) 0 2577 9009
E-mail : sumalee@tistr.or.th

เอกสารไม่ควบคุม



Request No. 25-67 / 0275

5 / 5

MTC. ACL. No. 358 / 67

3.7 Reading on wavelength- Nickel (Ni) at 232.0 nm.

Element	Standard Value of RM (mg/l)	Reading (mg/l)	Error of Measurement (mg/l)	Error of Measurement (%)	Uncertainty (mg/l)
Ni	0.101	0.098	-0.003	2.90	± 0.013
	0.508	0.502	-0.006	1.16	± 0.018
	1.012	0.962	-0.051	5.02	± 0.032

3.8 Reading on wavelength- Zinc (Zn) at 213.9 nm.

Element	Standard Value of RM (mg/l)	Reading (mg/l)	Error of Measurement (mg/l)	Error of Measurement (%)	Uncertainty (mg/l)
Zn	0.050	0.045	-0.005	9.39	± 0.013
	0.303	0.324	0.021	7.04	± 0.013
	0.707	0.675	-0.032	4.52	± 0.019

Remark : The reported uncertainty is an expanded uncertainty calculated using a coverage factor of 2 (k = 2)
which gives a level of confidence of approximately 95%

Calibrated by Atipat
(Mr. Atipat Ratana)

Approved by Sumalee
(Miss Suladda Deawong)
Director of Analytical Chemistry Laboratory
Issued Date : 11 March 2024

INDUSTRIAL METROLOGY AND TESTING SERVICE CENTRE
End of CertificateThe results relate only to the items tested/calibrated or value assigned.
Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BLMTC.002 Rev.4

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9000
Fax. (66) 0 2577 9009
E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

Office/Laboratory
Soi 1/C, Bangpoo Industrial Estate, Sukhumvit Road,
Amphoe Muang, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
Fax. (66) 0 2323 9165
E-mail : mtg@tistr.or.th

Office
196 Phahonyothin Road, Chatuchak, Bangkok 10900,
Thailand
Tel. (66) 0 2577 9000
Fax. (66) 0 2577 9009
E-mail : sumalee@tistr.or.th

เอกสารไม่ควบคุม

Agilent CrossLab Start Up Services

Agilent 5100 5110 ICP-OES Preventive Maintenance



Agilent Preventive Maintenance provides factory recommended service for your analytical instruments to assure reliable operation and the accuracy of your results

Delivered by highly trained and certified service engineers using genuine Agilent parts and supplies, Agilent Preventive Maintenance provides what you need to reduce unplanned downtime and keep your systems operating at their peak performance.

This checklist is used as a guide for completing the preventive maintenance tasks. A signed copy of this checklist is provided for your records.



เอกสารไม่ควบคุม

Introduction

Customer Information

- Customers should provide all necessary operating supplies upon request of the engineer.
- A customer representative should be available to the engineer while performing the preventive maintenance procedures. Customers are responsible for regular maintenance and are encouraged to observe the service representative.
- Any parts not included in the Parts Lists section of this document are not part of the recommended Preventive Maintenance service nor are they included in the price of this service.
- If a system requires the use of extra or special procedures and/or parts for the maintenance service, then these must be ordered separately and charged as a repair, which may incur additional costs.
- For customers using HF applications, the instrument should be returned to its standard sample introduction system.



เอกสารไม่ควบคุม



Important Customer Web Links

- To access **Agilent University**, visit <http://www.agilent.com/crosslab/university/> to learn about training options, which include online, classroom and onsite delivery. A training specialist can work directly with you to help determine your best options.
- To access the **Agilent Resource Center** web page, visit <https://www.agilent.com/en-us/agilentresources>. The following information topics are available:
 - Sample Prep and Containment
 - Chemical Standards
 - Analysis
 - Service and Support
 - Application Workflows
- The **Agilent Community** is an excellent place to get answers, collaborate with others about applications and Agilent products, and find in-depth documents and videos relevant to Agilent technologies. Visit <https://community.agilent.com/welcome>
- Videos about specific preparation requirements for your instrument can be found by searching the **Agilent YouTube** channel at <https://www.youtube.com/user/agilent>
- Need to place a service call?** [Flexible Repair Options | Agilent](#)



เอกสารไม่ควบคุม



Service Engineer's Responsibilities

- Contact the customer and ensure that all necessary supplies are available before the preventive maintenance visit.
- Only select those pages that relate to the system or module being serviced.
- Complete empty fields with the relevant information.
- Complete the relevant checkboxes in the checklist using either a "X" or tick mark "✓".
- Check **"Service not applicable"** check boxes to indicate services/tasks not delivered, as appropriate.
- Complete the Preventive Maintenance services in the most logical order relevant to the individual system service in the order of the tasks listed.
- Complete the **Service Review** section together with the customer.
- Complete the fields for page numbers at the foot of each selected page.
- Add relevant page numbers to selected pages and complete the total number of pages field in the Service Completion section
- Ask the customer to sign the Service Verification section including the customer's and your signature.**



เอกสารไม่ควบคุม

Instrument Maintenance

System Information

- ☐ Check this box if an instrument configuration report is attached instead of completing the table.

Instrument System Name and ID	5110 VDV ICP-OES
Instrument System Site and Location	United Analyst and Engineering Consultant

List System Component Product Numbers	List the Serial Numbers of each Component
1. G 805A	WY 19030001
2.	
3.	
4.	
5.	
6.	
7.	
8.	
9.	

ICP-OES Configuration Table	Circle the type or write in the type if other
Nebulizer Type	SeaSpray (OneNeb) Conical Other
Spray Chamber	Cyclonic Single Pass (Cyclonic Double Pass) Other
Torch	Radial (Dual View) Other
Torch Type	One Piece (Semi Demountable) Fully Demountable Other
Injector Diameter	2.4mm (1.8mm) 1.4mm 0.8mm Other
Injector Material	Quartz Ceramic Other

Preparation

- ☒ Discuss any specific issues with the customer before starting.
- ☒ Review the instrument logbook for recorded problems and comments.
- ☒ Save instrument control settings before starting the procedure.
- ☒ Perform a general inspection of the system for cleanliness.
- ☒ Check for proper installation of parts, assemblies, sensors etc.
- ☒ Check system for required installation of components and implementation of Service Notes
- ☒ Check for required firmware/software updates and verify with customers if they would like them installed.
- ☐ For HF application systems, if standard sample introduction system was not installed, ask the customer to install it. (N/A)
- ☒ Ask the customer to remove any samples from the ICP-OES sample introduction area, auto sampler or around the ICP-OES.

Preventive Maintenance Procedures

Record Pre-PM instrument performance

- ☒ Run Instrument Performance test.
- ☒ Record results in Instrument Performance Test Results Table – Pre-PM.

Clean and inspect ICP-OES system

- ☒ Look for any obvious external damage or problems.
- ☒ Inspect water cooling hoses, gas lines and power cord for excessive wear or damage.
- ☒ Perform a general internal inspection of the system for excessive dust accumulation, clean if necessary.
- ☒ Inspect sample introduction components and record any required maintenance in the Service Engineer Comments and notify the customer as the required actions required.
- ☒ Record the instrument operating conditions in the ICP-OES Status Results Table.
- ☒ Replace the polychromator purge filter.
- ☒ Replace the radial pre-optics window
- ☒ Replace the axial pre-optics window for SVDV and VDV instruments.
- ☒ Check exhaust flow for the correct positive extraction at the exhaust duct to insure they meet minimum specifications.
- ☒ Replace air inlet dust filter.
- ☐ Replace high capacity air inlet dust filter element if installed. (N/A)
- ☒ Remove and clean instrument water inlet filter.

Agilent Water Recirculator

- ☐ Service not applicable
- ☒ Drain cooling fluid and remove any particles from the chiller reservoir
- ☒ Remove, clean and reinstall water inlet metal mesh filter if present.
- ☒ Re fill with Agilent Cool Clear cooling fluid.
- ☒ Clean the cooling system Air filter and the condenser.

SPS 3 Auto Sampler

- ☒ Service not applicable
- ☐ Power cycle the autosampler and verify successful initialization.
- ☐ Inspect X and Z axis belts for wear. Replace is necessary.
- ☐ Clean X and Z axis slide shafts.
- ☐ Using customer's racks and the Agilent software move the sample probe to the 4 outermost corners and rinse probe, ensure that the probe is approximately centered in the vial.

SPS 4 Auto sampler

- ☒ Service not applicable
- ☐ Clean the spill tray, rack location mat, end frames and chassis with a damp soft cloth and diluted mild detergent.
- ☐ Clean the auto sampler cover panels, if cover kit is installed, with domestic window cleaner.
- ☐ Check the X-axis and Z-axis drive belts for cracks, splits, damaged teeth, excessive fraying, color changes or degradation from fumes.
- ☐ Check the X-axis, Theta-axis and Z-axis FFC cables for cracks, incorrect positioning, damaged edges or damaged connectors.
- ☐ Pump Tubing Replacement. Replace peristaltic pump tubing. Replace all tubing that goes from the rinse station to the pump and from the pump to the waste/rinse bottles
- ☐ Test using customer's tray and move the sample probe to the sample vial 1, wash vial and rinse port and ensure that the probe is centered in the vial. If not use calibration wizard and calibrate the position.

AVS 4, 6, 7 Advanced Valve System

- ☒ Service not applicable
- ☐ Replace valve rotor seal
- ☐ Check fittings for signs of leaks
- ☐ Check tubing including autosampler tubing for kinks or excessive wear
- ☐ Check high flow pump for signs of leaks

ICP-OES adjustment

- ☒ Check position of Zn peak, adjust if required.
- ☒ Check Argon Ratio, adjust to specified value if required.
- ☒ Perform Detector Calibration.
- ☒ Perform Instrument Calibration.

Record Post-PM instrument performance

- ☒ Run Instrument Performance test.
- ☒ Record results in Instrument Performance Test Results Table - Post PM.
- ☒ For systems using ICP Expert version 7.3 and above, run the following Instrument tests
 - ☒ Subsystem Communications Test
 - ☒ Air Flow
 - ☒ Water Flow
 - ☒ Gas Flows
 - ☒ RF Generator
 - ☒ Camera Test
 - ☒ Optics Test
 - ☒ Nebulizer Test

- ☒ Record the result in the Instrument Test Results Table

Test Results

Instrument Performance Test Results Table

Note: These measurements do not form part of any specification and are for reference only.

	Pre PM Sensitivity Check		Post PM Sensitivity Check	
	Radial	Axial *	Radial	Axial*
Zn 213.857 nm SRBR	1500.9	2219.4	4124.9	6965.9
Mn 257.610 nm SRBR	3915.0	7492.2	13017.6	31121.6
Al 396.152 nm SBR	9.7	10.7	9.7	21.1
K 766.491 nm SBR	6.7	28.1	4.8	45.3

* Axial result is not applicable for G8016AA, G8012AA Radial View instruments.

Instrument Test Results Table

Note: The Instrument Test results are for systems using ICP Expert version 7.3 and above only.

Instrument Test	Result
Subsystem Communications Test	Pass
Air Flow	Pass
Water Flow	Pass
Gas Flows	Pass
RF Generator	Pass
Camera Test	Pass
Optics Test	Pass
Nebulizer test	Pass

Restore Instrument

- ☐ For HF applications, ask the customer to reinstall their sample introduction system. N/A
- ☒ Leave system in an idle state: on and purging.
- ☒ Guidance: If the PM service is performed prior to a qualification service, then use the qualification procedure as a guide for final instrument set up and checkout.

Service Review

- ☒ Attach available reports/printouts of all tests to this documentation.
- ☒ Record the Preventive Maintenance service activity in the customer's records/logbook.
- ☒ Record the PM event in the Smart Alerts logbook, if applicable.
- ☒ Update/reset instrument maintenance counters as appropriate.
- ☒ Affix the PM sticker to the system or instrument logbook based on the customer's request.
- ☒ Complete the Service Engineer Comments section if there are additional comments.
- ☒ Review this service, parts replaced, and test results obtained with the customer.
- ☒ If the instrument firmware was updated, record the details of the change in the Service Engineer's Comments box. Systems in a compliant environment may need additional documentation.
- ☒ Complete the Signature Page with both Service Engineer and Customer signatures.

ICP-OES Status Results Table

Note: These measurements do not form part of any specification and are for reference only.

Measurement	Standby Mode	Plasma On
Mains Voltage	231.411 VAC	226.871 VAC
Mains Current	0.051 A	0.105 A
Instrument Temperature	22.1 °C	23.5 °C
RF Air Flow (sensor speed)	14.0 Hz	19.0 Hz
Plasma Exhaust Temperature	No measurement	63.6 °C
Water Flow Oscillator	No measurement	1.34 L/min
Water Flow Detector	0.86 L/min	0.81 L/min
Water Inlet Temperature	19.7 °C	19.7 °C
Polychromator Temperature	35.0 °C	35.0 °C
CCD Temperature	-40.1 °C	-39.6 °C
Thermal Stabilizer	35.0 °C	35.0 °C
Argon Supply Pressure	646.92 kPa	591.55 kPa
Purge Gas Supply Pressure*1	646.66 kPa	612.41 kPa
Option Gas Supply Pressure*1	— kPa	— kPa
Nebulizer Flow	No measurement	0.70 L/min
Nebulizer Back Pressure	No measurement	158.43 kPa
Plasma Gas Flow	No measurement	11.91 L/min
Auxiliary Gas Flow	No measurement	1.00 L/min
RF Power	No measurement	1204.7 W
RF Supply Current	No measurement	7.856 A
RF Supply Voltage	No measurement	204.417 V

*1 If option installed

Consumed PM Parts

Part Description	Part Number	Product or Model# where used	Quantity consumed
Axial Pre-Optic Window	G8010-68014	G8010A, G8011A, G8014A/G8015A	1
Radial Pre-Optic Window	G8010-68015	All	1
Agilent Cool Clear Coolant Fluid	5799-0037	Agilent Water Recirculator	-
Purge Gas Filter	G8010-60136	All	1
Air inlet filter	G8000-68002	All	1
High Capacity Air Filter	G8010-60189	Optional	-
Rotor seal for 6-7 port valve for AVS6/7	G8494-60002	G8494A/G8495	-
Rotor seal for 4 port valve for AVS4	G8493-60002	G8493A	-
Rinse solution to rinse station 2.5mm id x 1m	G8410-80123	SPS 4	-
Barb connector 2.5mm-1.5mm ID	G8410-80124	SPS 4	-
PVC waste tubing, 8mm od x 5mm id, 2m	G8410-80122	SPS 4	-
Additional Parts may be required from engineer's stock:			
X axis drive belt	5410047500	SPS 3	-
Z axis drive belt	5410047400	SPS 3	-
Peristaltic pump tubing, PVC SolvaFlex, 3 bridged,	3710049000	SPS 4	-

Consumed Parts Reference
(Purchased by customer, not included as part of PM)☒ Section Not Applicable

Part Description	Part Number	Product or Model# where used	Quantity consumed

Revision: A.02, Issued: 21 January 2022
Document Number: G8014-90075
© Agilent Technologies, Inc. 2022

Page 14 of 14



เอกสารไม่ควบคุม

Signature Page

Service Engineer Comments (optional)

If there are any specific points you wish to note as part of performing the installation or other items of interest for the customer, please write in this box.

Service Verification

Service Request Number:

6003197100

Date Service Completed:

04 Nov 2024

Service Engineer Name:

Kanyakorn S.

Customer Name:

Aphorn Onkong

Service Engineer Signature:

Kanyakorn S.

Customer Signature:

Aphorn Onkong

Total number of pages in this document:

14

Revision: A.02, Issued: 21 January 2022
Document Number: G8014-90075
© Agilent Technologies, Inc. 2022

Page 14 of 14



เอกสารไม่ควบคุม

Report Summary

Instrument Model Agilent 5100/5110 VDV ICP-OES
Instrument ID G8011A/G8015A
Instrument Serial Number MY18030001
Software Version 7.3.1.9507
Firmware Version 3442
Tested By Pre Test_PM_Kanyakorn S.
Test Completed On 11/4/2024 9:19:10 AM

Result Summary

Subsystem Communications Test	Skipped
Air Flow Test	Skipped
Water Flow Test	Skipped
Gas Flows Test	Skipped
RF Generator Test	Skipped
Camera Test	Skipped
Optics Test	Skipped
Advanced Valve System Test	Skipped
Resolution Test	Pass
Sensitivity Test	Fail
Precision Test	Pass

Page 1 of 4

เอกสารไม่ควบคุม

Resolution Test

Pass

Element Wavelength	Specification	Width
N (174.213 nm)	≤ 9.40	6.98
As (188.980 nm)	≤ 8.20	6.17
C (193.027 nm)	≤ 11.50	8.30
Mo (202.032 nm)	≤ 8.20	6.38
Cr (206.158 nm)	≤ 13.40	8.98
Zn (213.857 nm)	≤ 8.70	6.60
Pb (220.353 nm)	≤ 9.50	7.09
Co (228.615 nm)	≤ 17.20	11.67
Ba (230.424 nm)	≤ 9.40	7.20
Mn (257.610 nm)	≤ 13.30	9.43
Mn (260.568 nm)	≤ 20.30	14.11
Cr (267.716 nm)	≤ 11.00	8.04
Cu (324.754 nm)	≤ 25.00	18.97
Cu (327.395 nm)	≤ 14.20	11.23
Sr (338.071 nm)	≤ 33.50	24.30
Ba (455.403 nm)	≤ 44.00	33.47
Sr (460.733 nm)	≤ 36.00	17.23
Ba (493.408 nm)	≤ 36.00	25.37
Ba (614.171 nm)	≤ 42.00	25.54
Ar (675.283 nm)	≤ 74.00	56.51
K (766.491 nm)	≤ 80.00	65.86

Page 2 of 4

เอกสารไม่ควบคุม

Sensitivity Test			Fail		
Radial					
Element Wavelength	Specification	Method	Ratio	Standard	Blank
As (188.980 nm)	≥ 46.0	SRBR	104.1	793.0	50.8
Se (196.026 nm)	≥ 41.0	SRBR	87.6	862.0	79.7
Zn (213.857 nm)	≥ 1421.0	SRBR	1500.8	41823.3	749.0
Pb (220.353 nm)	≥ 46.0	SRBR	170.7	2432.0	174.9
Mn (257.610 nm)	≥ 3518.0	SRBR	3915.0	264700.2	4420.0
Al (396.152 nm)	≥ 3.4	SBR	7.7	48454.6	5563.2
Ba (493.408 nm)	≥ 34.0	SBR	45.9	1966719.7	41903.8
K (766.491 nm)	≥ 1.8	SBR	5.7	99038.2	14687.7
Axial					
Element Wavelength	Specification	Method	Ratio	Standard	Blank
As (188.980 nm)	≥ 208.0	SRBR	126.5	1498.8	119.0
Se (196.026 nm)	≥ 159.0	SRBR	112.0	1773.6	197.8
Zn (206.200 nm)	≥ 234.0	SRBR	466.0	6784.2	199.7
Zn (213.857 nm)	≥ 1743.0	SRBR	2217.4	95597.6	1789.7
Cd (214.439 nm)	≥ 4227.0	SRBR	1919.3	68724.6	1236.4
Pb (220.353 nm)	≥ 320.0	SRBR	332.6	7929.5	499.0
Mn (257.610 nm)	≥ 10625.0	SRBR	7492.2	991238.3	16911.7
Cr (267.716 nm)	≥ 1048.0	SRBR	2254.6	129706.6	3150.9
Cu (324.754 nm)	≥ 19.0	SBR	26.9	290746.3	10407.5
Al (396.152 nm)	≥ 6.0	SBR	10.7	211329.2	18005.0
Ba (493.408 nm)	≥ 60.0	SBR	49.3	6956460.4	138336.9
K (766.491 nm)	≥ 24.0	SBR	28.1	1395190.2	47996.2

Page 3 of 4

เอกสารไม่ควบคุม

Precision Test			Pass
Radial			
Element Wavelength	Specification	Measured Value % RSD	
As (188.980 nm)	≤ 2.60	0.73	
Se (196.026 nm)	≤ 2.60	0.95	
Zn (213.857 nm)	≤ 1.50	0.31	
Pb (220.353 nm)	≤ 2.60	0.73	
Mn (257.610 nm)	≤ 1.50	0.39	
Al (396.152 nm)	≤ 1.50	0.39	
Ba (493.408 nm)	≤ 1.50	0.87	
K (766.491 nm)	≤ 1.50	0.32	
Axial			
Element Wavelength	Specification	Measured Value % RSD	
As (188.980 nm)	≤ 1.50	1.21	
Se (196.026 nm)	≤ 1.50	0.84	
Zn (206.200 nm)	≤ 1.50	0.56	
Zn (213.857 nm)	≤ 1.50	0.96	
Cd (214.439 nm)	≤ 1.50	0.26	
Pb (220.353 nm)	≤ 1.50	0.51	
Mn (257.610 nm)	≤ 1.50	0.97	
Cr (267.716 nm)	≤ 1.50	0.22	
Cu (324.754 nm)	≤ 1.50	0.24	
Al (396.152 nm)	≤ 1.50	0.33	
Ba (493.408 nm)	≤ 1.50	0.40	
K (766.491 nm)	≤ 1.50	0.65	

Page 4 of 4

เอกสารไม่ควบคุม

Report Summary	
Instrument Model	Agilent 5100/5110 VDV ICP-OES
Instrument ID	G8011A/G8015A
Instrument Serial Number	MY18030001
Software Version	7.3.1.9507
Hardware Version	3442
Tested By	Post Test_PM_Kanyakorn S.
Test Completed On	11/4/2024 11:07:24 AM
Result Summary	
Subsystem Communications Test	Pass
Air Flow Test	Skipped
Water Flow Test	Skipped
Gas Flows Test	Skipped
RF Generator Test	Skipped
Camera Test	Skipped
Optics Test	Pass
Advanced Valve System Test	Skipped
Resolution Test	Pass
Sensitivity Test	Fail
Precision Test	Pass
Subsystem Communications Test	Pass
Optics Test	Pass
Intensity	3184054
Wavelength	737.212

Page 1 of 4

เอกสารไม่ควบคุม

Resolution Test			Pass		
Element Wavelength	Specification	Width			
N (174.213 nm)	≤ 9.40	6.97			
As (188.980 nm)	≤ 8.20	6.14			
C (193.027 nm)	≤ 11.50	8.33			
Mo (202.032 nm)	≤ 8.20	6.33			
Cr (206.133 nm)	≤ 13.40	9.06			
Zn (213.637 nm)	≤ 8.70	6.70			
Pb (220.353 nm)	≤ 9.50	7.03			
Co (228.615 nm)	≤ 17.20	11.72			
Ba (230.424 nm)	≤ 9.40	7.32			
Mn (257.610 nm)	≤ 13.30	9.44			
Mn (260.568 nm)	≤ 20.30	14.21			
Cr (267.716 nm)	≤ 11.00	7.94			
Cu (324.754 nm)	≤ 25.00	18.99			
Cu (327.395 nm)	≤ 14.20	11.27			
Sr (338.071 nm)	≤ 33.50	24.40			
Ba (455.403 nm)	≤ 44.00	33.50			
Sr (460.793 nm)	≤ 36.00	17.31			
Ba (493.408 nm)	≤ 36.00	25.44			
Ba (614.171 nm)	≤ 42.00	25.16			
Ar (675.283 nm)	≤ 74.00	56.15			
K (766.491 nm)	≤ 80.00	65.56			

Page 2 of 4

เอกสารไม่ควบคุม

Sensitivity Test					
Fail					
Radial					
Element Wavelength	Specification	Method	Ratio	Standard	Blank
As (188.980 nm)	≥ 46.0	SRBR	130.6	977.1	50.4
Se (196.026 nm)	≥ 41.0	SRBR	106.0	958.7	70.2
Zn (213.857 nm)	≥ 1421.0	SRBR	4124.8	44037.7	113.4
Pb (220.353 nm)	≥ 46.0	SRBR	207.2	2554.7	136.2
Mn (257.610 nm)	≥ 3518.0	SRBR	13017.8	271846.6	434.7
Al (396.152 nm)	≥ 3.4	SBR	9.7	50615.5	4717.0
Ba (493.408 nm)	≥ 34.0	SBR	133.7	2069203.0	15359.3
K (766.491 nm)	≥ 1.8	SBR	4.8	100199.5	17235.5
Axial					
Element Wavelength	Specification	Method	Ratio	Standard	Blank
As (188.980 nm)	≥ 208.0	SRBR	174.9	1566.7	73.0
Se (196.026 nm)	≥ 159.0	SRBR	167.0	1863.4	110.2
Zn (206.200 nm)	≥ 234.0	SRBR	740.9	6836.0	83.1
Zn (213.857 nm)	≥ 1743.0	SRBR	6965.9	101568.1	211.7
Cd (214.439 nm)	≥ 4227.0	SRBR	5781.0	72852.9	158.1
Pb (220.353 nm)	≥ 320.0	SRBR	501.0	8464.3	267.7
Mn (257.610 nm)	≥ 10625.0	SRBR	31121.6	1006637.8	1044.0
Cr (267.716 nm)	≥ 1048.0	SRBR	4424.8	132202.9	880.8
Cu (324.754 nm)	≥ 19.0	SBR	68.7	302907.8	4345.6
Al (396.152 nm)	≥ 6.0	SBR	21.1	218771.0	9892.3
Ba (493.408 nm)	≥ 60.0	SBR	250.6	7137380.9	28367.3
K (766.491 nm)	≥ 24.0	SBR	45.3	1435050.6	31025.0

Page 3 of 4

เอกสารไม่ควบคุม

Precision Test					
Pass					
Radial					
Element Wavelength	Specification	Measured Value	% RSD		
As (188.980 nm)	≤ 2.60	0.81			
Se (196.026 nm)	≤ 2.60	0.98			
Zn (213.857 nm)	≤ 1.50	0.22			
Pb (220.353 nm)	≤ 2.60	0.37			
Mn (257.610 nm)	≤ 1.50	0.27			
Al (396.152 nm)	≤ 1.50	0.25			
Ba (493.408 nm)	≤ 1.50	0.53			
K (766.491 nm)	≤ 1.50	0.15			
Axial					
Element Wavelength	Specification	Measured Value	% RSD		
As (188.980 nm)	≤ 1.50	0.81			
Se (196.026 nm)	≤ 1.50	0.65			
Zn (206.200 nm)	≤ 1.50	0.79			
Zn (213.857 nm)	≤ 1.50	0.81			
Cd (214.439 nm)	≤ 1.50	0.35			
Pb (220.353 nm)	≤ 1.50	0.33			
Mn (257.610 nm)	≤ 1.50	1.02			
Cr (267.716 nm)	≤ 1.50	0.32			
Cu (324.754 nm)	≤ 1.50	0.51			
Al (396.152 nm)	≤ 1.50	0.37			
Ba (493.408 nm)	≤ 1.50	0.68			
K (766.491 nm)	≤ 1.50	0.74			

Page 4 of 4

เอกสารไม่ควบคุม

Report Summary		
Instrument Model	Agilent 5100/5110 VDV ICP-OES	
Instrument ID	G8011A/G8015A	
Instrument Serial Number	MY18030001	
Software Version	7.3.1.9507	
Firmware Version	3442	
Tested By	Post Test_PM_Kanyakorn S.	
Test Completed On	11/4/2024 11:30:15 AM	
Result Summary		
Subsystem Communications Test		Pass
Air Flow Test		Pass
Water Flow Test		Pass
Gas Flows Test		Pass
RF Generator Test		Pass
Camera Test		Pass
Optics Test		Skipped
Advanced Valve System Test		Skipped
Resolution Test		Skipped
Sensitivity Test		Skipped
Precision Test		Skipped
Subsystem Communications Test		Pass
Air Flow Test		Pass
30% Air Flow (relative speed)	75% Air Flow (relative speed)	
15.00	19.00	
Water Flow Test		Pass
RF Water Flow(L/min)	Camera Water Flow (L/min)	Water Inlet Temperature (°C)
1.30	0.81	20.55

Page 1 of 2

เอกสารไม่ควบคุม

Gas Flows Test					
Pass					
Nebulizer Target Flow	Actual Flow	Back Pressure	Auxiliary Target Flow	Actual Flow	Back Pressure
0.70	0.70	154.65	2.00	2.00	110.92
Makeup Target Flow	Actual Flow	Back Pressure	Plasma Target Flow	Actual Flow	Back Pressure
2.00	2.00	115.38	18.00	17.97	21.48
RF Generator Test					
Pass					
RF Power Supply Test	Passed				
RF Power Supply (V)	128.554				
RF Oscillator Test	Passed				
RF Oscillator Frequency (MHz)	25.834				
Work Coil Current (A)	44.660				
RF Power Supply Current (A)	1.999				
Camera Test					
Pass					
	Integration Time (ms)	Standard Deviation	Status		
Electronic Offset Test	1000	5.228	Passed		
Dark Current Test	6000	1.168	Passed		
Array Test	5	0.024	Passed		
Linearity Test		0.118	Passed		

Page 2 of 2

เอกสารไม่ควบคุม

Report Summary	
Instrument Model	Agilent 5100/5110 VDV ICP-OES
Instrument ID	G8011A/G8015A
Instrument Serial Number	MY18030001
Software Version	7.3.1.9507
Firmware Version	3442
Tested By	change mirror
Test Completed On	11/6/2024 10:35:26 AM
Result Summary	
Subsystem Communications Test	Skipped
Air Flow Test	Skipped
Water Flow Test	Skipped
Gas Flows Test	Skipped
RF Generator Test	Skipped
Camera Test	Skipped
Optics Test	Skipped
Advanced Valve System Test	Skipped
Resolution Test	Pass
Sensitivity Test	Pass
Precision Test	Pass

Page 1 of 4

เอกสารไม่ควบคุม

Resolution Test			Pass
Element Wavelength	Specification	Width	
N (174.213 nm)	≤ 9.40	6.79	
As (188.980 nm)	≤ 8.20	5.80	
C (193.027 nm)	≤ 11.50	8.15	
Mo (202.032 nm)	≤ 8.20	5.90	
Cr (206.158 nm)	≤ 13.40	8.85	
Zn (213.857 nm)	≤ 8.70	6.77	
Pb (220.353 nm)	≤ 9.50	6.61	
Co (228.615 nm)	≤ 17.20	11.79	
Ba (230.424 nm)	≤ 9.40	7.25	
Mn (257.610 nm)	≤ 13.30	9.47	
Mn (260.568 nm)	≤ 20.30	14.50	
Cr (267.716 nm)	≤ 11.00	7.91	
Cu (324.754 nm)	≤ 25.00	18.72	
Cu (327.395 nm)	≤ 14.20	11.09	
Sr (338.071 nm)	≤ 33.50	25.39	
Ba (455.403 nm)	≤ 44.00	33.09	
Sr (460.733 nm)	≤ 36.00	18.54	
Ba (493.408 nm)	≤ 36.00	25.74	
Ba (614.171 nm)	≤ 42.00	25.23	
Ar (675.283 nm)	≤ 74.00	58.92	
K (766.491 nm)	≤ 80.00	63.16	

Page 2 of 4

เอกสารไม่ควบคุม

Sensitivity Test						Pass
Radial						
Element Wavelength	Specification	Method	Ratio	Standard	Blank	
As (188.980 nm)	≥ 46.0	SRBR	110.5	868.9	54.3	
Se (196.026 nm)	≥ 41.0	SRBR	88.3	934.7	91.3	
Zn (213.857 nm)	≥ 1421.0	SRBR	3535.4	44017.7	153.9	
Pb (220.353 nm)	≥ 46.0	SRBR	184.5	2492.3	159.8	
Mn (257.610 nm)	≥ 3518.0	SRBR	11099.6	249595.3	503.6	
Al (396.152 nm)	≥ 3.4	SBR	8.7	50274.4	5172.0	
Ba (493.408 nm)	≥ 34.0	SBR	124.5	1903164.1	15166.0	
K (766.491 nm)	≥ 1.8	SBR	6.9	110041.4	13991.2	
Axial						
Element Wavelength	Specification	Method	Ratio	Standard	Blank	
As (188.980 nm)	≥ 208.0	SRBR	253.3	3744.3	196.3	
Se (196.026 nm)	≥ 159.0	SRBR	206.7	4199.7	347.2	
Zn (206.200 nm)	≥ 234.0	SRBR	923.0	12282.3	172.1	
Zn (213.857 nm)	≥ 1743.0	SRBR	6398.3	157551.5	601.7	
Cd (214.439 nm)	≥ 4227.0	SRBR	5069.2	99873.7	385.2	
Pb (220.353 nm)	≥ 320.0	SRBR	389.0	10641.1	658.6	
Mn (257.610 nm)	≥ 10625.0	SRBR	21190.4	985528.7	2153.6	
Cr (267.716 nm)	≥ 1048.0	SRBR	3054.1	131797.6	1811.5	
Cu (324.754 nm)	≥ 19.0	SBR	36.3	301401.4	8082.9	
Al (396.152 nm)	≥ 6.0	SBR	10.8	228359.5	19280.5	
Ba (493.408 nm)	≥ 60.0	SBR	106.5	6460421.5	60122.8	
K (766.491 nm)	≥ 24.0	SBR	30.2	1639840.6	52562.1	

Page 3 of 4

เอกสารไม่ควบคุม

Precision Test			Pass
Radial			
Element Wavelength	Specification	Measured Value % RSD	
As (188.980 nm)	≤ 2.60	1.56	
Se (196.026 nm)	≤ 2.60	1.16	
Zn (213.857 nm)	≤ 1.50	0.50	
Pb (220.353 nm)	≤ 2.60	0.74	
Mn (257.610 nm)	≤ 1.50	0.63	
Al (396.152 nm)	≤ 1.50	0.54	
Ba (493.408 nm)	≤ 1.50	0.78	
K (766.491 nm)	≤ 1.50	0.44	
Axial			
Element Wavelength	Specification	Measured Value % RSD	
As (188.980 nm)	≤ 1.50	0.82	
Se (196.026 nm)	≤ 1.50	0.82	
Zn (206.200 nm)	≤ 1.50	0.35	
Zn (213.857 nm)	≤ 1.50	0.34	
Cd (214.439 nm)	≤ 1.50	0.44	
Pb (220.353 nm)	≤ 1.50	0.48	
Mn (257.610 nm)	≤ 1.50	0.83	
Cr (267.716 nm)	≤ 1.50	0.53	
Cu (324.754 nm)	≤ 1.50	0.69	
Al (396.152 nm)	≤ 1.50	0.56	
Ba (493.408 nm)	≤ 1.50	1.29	
K (766.491 nm)	≤ 1.50	0.74	

Page 4 of 4

เอกสารไม่ควบคุม

List of Instruments Certification for Air & Noise Quality Analysis

No.	Instrument/Equipment	Parameter	Manufacturer	Model/Serial No.	Calibrator	Certification No.	Date of Calibration	Due date of Calibration	Remark
Stack									
1	Pre-Test Console	Total Suspended Particulate	Apex Instruments, USA.	XC-572-V 1701019	Envi Equipment Service Co., Ltd.	E24-060048	18 Jun 24	17 Jun 25	-
2	Flue gas Analyzer	Sulphur Dioxide Oxide of Nitrogen as Nitrogen Dioxide	Testo	Testo 350 60899698/701	Entech Industrial Solution Co., Ltd.	G 670083	8 Feb 24	7 Feb 25	-

List of Instruments Certification for Air & Noise Quality Analysis

No.	Instrument/Equipment	Parameter	Manufacturer	Model/Serial No.	Calibrator	Certification No.	Date of Calibration	Due date of Calibration	Remark
Ambient									
1	Orifice Transfer Standard Calibrator	Total Suspended Particulate (TSP) Particulate Matter < 10 µm (PM ₁₀)	Andersen Instruments, Inc.	G25A 1901	Jiranatee Associates Co., Ltd.	COF-032-67	17 Jul 24	16 Jul 25	-
2	U-Tube Manometer	Total Suspended Particulate (TSP) Particulate Matter < 10 µm (PM ₁₀)	Dwyer	1221-36-W/M -	Technology Promotion Association (Thailand-Japan)	24P1251	11 Apr 24	10 Apr 25	-
3	Aneroid Barometer	Total Suspended Particulate (TSP) Particulate Matter < 10 µm (PM ₁₀)	Barigo, Germany	-	Technology Promotion Association (Thailand-Japan)	24P1369	22 Apr 24	21 Apr 25	-
4	Dial Thermo-Hygrometer	Total Suspended Particulate (TSP) Particulate Matter < 10 µm (PM ₁₀)	Barigo, Germany	-	Technology Promotion Association (Thailand-Japan)	24H753	10 Apr 24	9 Apr 25	-
5	Nitrogen Dioxide Analyzer	Nitrogen Dioxide	Thermo Scientific	42i CM08130002	UAE Consultant Co.,Ltd.	17092024	17 Sep 24	16 Sep 25	-
6	Nitrogen Dioxide Analyzer	Nitrogen Dioxide	Thermo Scientific	42i CM19050148	UAE Consultant Co.,Ltd.	20092024	20 Sep 24	19 Sep 25	-
7	Nitrogen Dioxide Analyzer	Nitrogen Dioxide	Thermo Scientific	42i CM19050149	UAE Consultant Co.,Ltd.	17092024	17 Sep 24	16 Sep 25	-
8	Standard Gases (Mixture)	Nitrogen Dioxide	Airgas	EB0162121 2016PSIG	Airgas an Air Liquide company	E05NI91E15A0014	6 Jun 23	6 Jun 31	-
9	Sulphur Dioxide Analyzer	Sulphur Dioxide	Thermo Scientific	43i CM22387061	UAE Consultant Co.,Ltd.	06092024	6 Sep 24	5 Sep 25	-
10	Sulphur Dioxide Analyzer	Sulphur Dioxide	Thermo Scientific	43i CM22387063	UAE Consultant Co.,Ltd.	19062024	19 Jun 24	18 Jun 25	-
11	Sulphur Dioxide Analyzer	Sulphur Dioxide	Thermo Scientific	43i CM22387067	UAE Consultant Co.,Ltd.	15052024	15 May 24	14 May 25	-
12	Standard Gases (Mixture)	Nitrogen Dioxide	Airgas	EB0162121 2016PSIG	Airgas an Air Liquide company	E05NI91E15A0014	6 Jun 23	6 Jun 31	-
13	Sound Level Calibrator (Acoustic Calibrator)	Calibrate Sound Level Meter	Svantek	SV36 107224	Innovative Instrument Co.,Ltd.	24-ACT-091	26 Jun 24	25 Jun 25	-

List of Instruments Certification for Air & Noise Quality Analysis

No.	Instrument/Equipment	Parameter	Manufacturer	Model/Serial No.	Calibrator	Certification No.	Date of Calibration	Due date of Calibration	Remark
Ambient									
14	Sound Level Meter	$L_{Aeq\ 1\ hour}$, $L_{Aeq\ 24\ hrs}$, L_{Amax} , L_{A90}	Larson Davis	LxT2	Electrical And Electronics Institute Foundation For Industrial Development	CP20240292EA	6 Aug 24	5 Aug 25	-
				0005348					
15	Sound Level Meter	$L_{Aeq\ 1\ hour}$, $L_{Aeq\ 24\ hrs}$, L_{Amax} , L_{A90}	Larson Davis	LxT2	Innovative Instrument Co.,Ltd.	24-SLM-237	10 Jul 24	9 Jul 25	-
				0005393					
16	Sound Level Meter	$L_{Aeq\ 1\ hour}$, $L_{Aeq\ 24\ hrs}$, L_{Amax} , L_{A90}	Larson Davis	LxT2	Electrical And Electronics Institute Foundation For Industrial Development	CP20240291EA	5 Aug 24	4 Aug 25	-
				0005396					

List of Instruments Certification for Water Quality Analysis

No.	Instrument/Equipment	Parameter	Manufacturer	Model/Serial No.	Calibrator	Certification No.	Date of Calibration	Due date of Calibration	Remark
Water									
1	pH Meter	pH	Horiba	LAQUA-PH210	Technology Promotion Association (Thailand-Japan)	24CH239	20 Feb 24	19 Feb 25	-
				HA0D0078					

CERTIFICATE OF CALIBRATION

Customer : United Analyst and Engineering Consultant Co., Ltd.

Address : 81 Soi Udomsuk 41, Sukhumvit Road, Banghak, Phrakhanong, Bangkok 10260

Description of Equipment : Console meter

Manufacturer : Apex Instrument

Model Number : XC-572-V

Serial Number : 1701019

ID/Control No. : UAE.EFM 013/2560

Environment Conditions : Temperature (25 ± 2) °C
Humidity (50 ± 15) % RH

Cal. Date : 18/06/2024

Issue Date : 18/06/2024

Calibration Method or Calibration Procedure Used

US EPA Method (United State Environmental Protection Agency)

This certificate is traceable to national standard, which realize the units of measurement according to the International System of Units (SI).

Result of Calibration

This certificate may not be reproduced other than in full except with prior Written approval of the Technical Manager, Envi Equipment Service Company Limited.

These reported uncertainties of measurement are expanded by a coverage factor of k=2, providing a 95% confidence level

Calibrated by : Mr. Sanya Sangnil

Approved by :

(Mr. Mana Fuchnoi)

Technical Manager

เอกสารไม่ควบคุม

METHOD 5 CONSOLE CALIBRATION
USING REFERENCE WET GAS METER W-NK-2.5-B-Z No.547425
5-POINT METRIC UNIT

Meter Console Information		Calibration Conditions				Factors/Conversions		
Console Model Number	XC-572-V	Date	Time	18/06/2024	10:00 AM	Std Temp	293	K
Console Serial Number	1701019	Calibration Reference No.	SER24-060018			Std Press	760	mm Hg
DGM Model Number	SK2SEX	Barometric Pressure	755.91	mmHg		K ₁	0.386	
DGM Serial Number	00002028	Calibration Meter Gamma	1.001			Console Leak Check	PASS	

Calibration Data									
Run Time		Metering Console					Calibration Meter		
Elapsed	DGM Orifice DH	Volume Initial	Volume Final	Outlet Temp Initial	Outlet Temp Final	Volume Initial	Volume Final	Outlet Temp Initial	Outlet Temp Final
(Q)	(P ₀)	(V _{in})	(V _{out})	(t _{in})	(t _{out})	(V _{in})	(V _{out})	(t _{in})	(t _{out})
min	mm H ₂ O	m ³	m ³	°C	°C	m ³	m ³	°C	°C
11.82	13.0	2802.112	2802.252	32	32	222.03382	222.17160	29	29
11.85	13.0	2802.252	2802.392	32	32	222.17160	222.30948	29	29
8.42	26.0	2802.399	2802.539	32	32	222.31644	222.45472	29	29
8.43	26.0	2802.539	2802.679	32	32	222.45472	222.59264	29	29
13.80	40.0	2802.686	2802.966	32	32	222.59970	222.87558	28	28
13.78	48.0	2802.966	2803.246	32	32	222.87558	223.15024	27	27
10.32	70.0	2803.261	2803.541	33	33	223.16476	223.43840	27	27
10.33	70.0	2803.541	2803.821	33	33	223.43840	223.71148	27	27
9.00	90.0	2803.835	2804.115	33	33	223.72450	223.99668	27	27
9.00	90.0	2804.115	2804.395	33	33	223.99668	224.26896	27	27



เอกสารไม่ควบคุม

METHOD 5 CONSOLE CALIBRATION
USING REFERENCE WET GAS METER W-NK-2.5-B-Z No.547425
5-POINT METRIC UNIT

Meter Console Information		Calibration Conditions				Factors/Conversions		
Console Model Number	XC-572-V	Date	Time	18/06/2024	10:00 AM	Std Temp	293	K
Console Serial Number	1701019	Calibration Reference No.	SER24-060018			Std Press	760	mm Hg
DGM Model Number	SK2SEX	Barometric Pressure	755.91	mmHg		K ₁	0.386	
DGM Serial Number	00002028	Calibration Meter Gamma	1.001			Console Leak Check	PASS	


Calibration Data									
Results									
Standardized Data					Dry Gas Meter				
Dry Gas Meter		Calibration Meter		Calibration Factor	Variation	Flowrate		Variation	Variation
(V _{std})	(Q _{std})	(V _{wet})	(Q _{wet})			Std & Corr	(Q _{std})		
m ³	m ³ /min	m ³	m ³ /min	(Y)	(ΔY)	(Q _{std})	(ΔH _g)	(ΔH _g)	(ΔH _g)
0.135	0.011	0.133	0.011	0.984	0.007	0.011	44.706	-1.370	
0.135	0.011	0.133	0.011	0.985	0.008	0.011	44.893	-1.182	
0.135	0.016	0.134	0.016	0.986	0.009	0.016	45.148	-0.928	
0.135	0.016	0.133	0.016	0.984	0.007	0.016	45.564	-0.512	
0.272	0.020	0.267	0.019	0.982	0.005	0.019	46.883	0.808	
0.273	0.020	0.267	0.019	0.978	0.001	0.019	47.030	0.954	
0.274	0.027	0.266	0.026	0.972	-0.005	0.026	46.723	0.648	
0.274	0.027	0.266	0.026	0.970	-0.007	0.026	47.067	0.991	
0.274	0.030	0.265	0.029	0.965	-0.012	0.029	46.388	0.313	
0.274	0.030	0.265	0.029	0.965	-0.012	0.029	46.354	0.279	
0.977				Y Average			46.075	ΔH _g Average	

Note: For Calibration Factor Y, the ratio of the reading of the calibration meter to the dry gas meter, acceptable tolerance of individual values from the average is ±0.02.

For ΔH_g, orifice pressure differential that equates to 0.75 cm (0.0212 m³/min) at standard temperature and pressure, acceptable tolerance of individual values from the average is ±0.2 inches (5.1mm).

เอกสารไม่ควบคุม

Meter Console Information		Calibration Conditions				Factors/Conversions		
Console Model Number	XC-572-V	Date	Time	18/06/2024	10:00 AM	Std Temp	293	K
Console Serial Number	1701019	Calibration Reference No.	SER24-060018			Std Press	760	mm Hg
DGM Model Number	SK2SEX	Barometric Pressure	755.91	mmHg		K ₁	0.386	
DGM Serial Number	00002028	Calibration Meter Gamma	1.001			Console Leak Check	PASS	

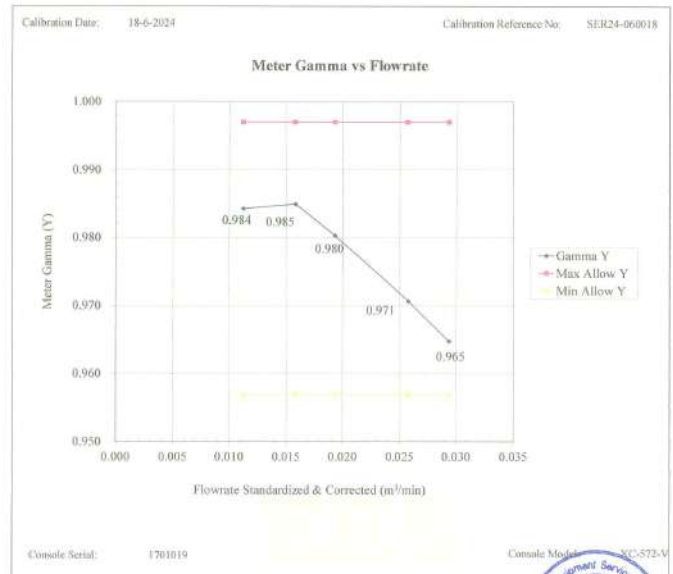

เอกสารไม่ควบคุม

Meter Console Information		Calibration Conditions				Factors/Conversions		
Console Model Number	XC-572-V	Date	Time	18/06/2024	10:00 AM	Std Temp	293	K
Console Serial Number	1701019	Calibration Reference No.	SER24-060018			Std Press	760	mm Hg
DGM Model Number	SK25EX	Barometric Pressure	755.91 mmHg			K ₁	0.386	
DGM Serial Number	00002028	Calibration Meter Gamma	1.001			Console Leak Check	PASS	



เอกสารไม่ควบคุม

THERMOCOUPLES SYSTEM CALIBRATION

Sampling System Equipment Information		Calibration Conditions	
Console Model Number	XC-572-V	Date	Time
Console Serial Number	1701019	18/06/2024	00:20 PM
DGM Model Number	SK25EX	Calibration Reference No.	SER24-060018
DGM Serial Number	00002028	Reference Thermometer	DIGICON
Meter Box Model Number	JENCO 765 KF	Serial Number	183169105
Meter Box Serial Number	JC 19777		

Results	
Console Thermocouple Simulator	
Channel and test point	Meter Box Channel Temperature Reading (°C)
	-18.0 25.0 38.0 93.0 149.0 260.0 371.0 482.0 593.0 816.0 1038.0
Stack	-17.0 25.0 38.0 93.0 149.0 257.0 368.0 477.0 587.0 806.0 1024.0
Aux	-17.0 25.0 38.0 93.0 149.0
Probe	-17.0 25.0 38.0 93.0 149.0
Filter	-17.0 25.0 38.0 93.0 149.0
Oven	-17.0 25.0 38.0 93.0 149.0
Exit	-17.0 25.0 38.0

Tolerance Range	
Stack	± 1.50% Absolute
Probe	± 3.0 °C
Filter	± 3.0 °C
Meter	± 3.0 °C
Exit	± 2.0 °C



เอกสารไม่ควบคุม

Certificate No: G 670083
Date of issue : 08-Feb-24

Instrument description	Flue Gas Analyzer
Instrument model	Testo 350 New
Control unit serial no.	03099393/701
Instrument serial no.	60899698/701
ID no. or control no.	UAE.EPM.008/2560
Manufacturer	Testo SE & Co. KGaA
Probe description	-
Probe model	-
Probe serial no.	-
Customer name	UNITED ANALYST CONSULTANT CO.,LTD.
Customer address	81 SOI UDOMSUK41, SUKHUMVIT ROAD, BANGOCHAK PRAKONG BANGKOK 10260

Total pages of certificate	2 Pages
Receiving no.	L-240430
Receiving date.	05-Feb-24
Parameter of calibration	Gas Calibration(Oxygen 2.50,10.04,21.02 %vol, Carbon Monoxide 80.14,302,1003 ppm, Nitrogen Dioxide 30.34,81.32, 201.9 ppm, Nitric Oxide 30.01, 151.5, 322.5 ppm, Sulphur Dioxide 50.36, 100.8, 600.8 ppm)
Condition of UUC.	Used
Ambient condition	All of the Measurement were carried out the stabilized laboratory Temperature : 23 ± 5 °C Humidity : 55 ± 15 %RH
Calibration place	17/121 Soi Ngamwongwan 47 Yaek 48, Toongsonghong, Lakse, Bangkok 10210
Calibration procedure no.	This instrument was calibrated by comparison with Standard gas mixture according to calibration Work Instruction no. WI-CL-28-C.

The calibration certificate expanded uncertainty of measurement is stated as the standard uncertainty of measurement Multiplied by coverage factor $k=2$, which for a normal distribution corresponds to a coverage probability of approximately 95%. This certificate is applied only to item under test Environmental condition.

This Calibration Certificate may not be reproduced other than in full except with the permission of the issuing laboratory.

Calibration certificates without signature and seal not valid and The results relate only to the items tested/calibrated.

This calibration certificate documents are traceability to national standards, which realize measurement according to the International System of Units (SI).

Date of calibration : 08-Feb-24

Mr. Kwanchai Khamsoung
Calibration Technician

Mrs. Nongluck Wongsettee
Technical Manager

เอกสารไม่ควบคุม

Certificate No.: G 670083

Standard References (Table 1)

Standard	Certificate No.	Vendor	Due date
Oxygen (O ₂) 2.50 % Vol	2412/23	Linde	27-Aug-27
Oxygen (O ₂) 10.04 % Vol	CG-0153-21	Nimt	18-Nov-26
Oxygen (O ₂) 21.02 % Vol	CG-0041-22	Nimt	10-Feb-27
Carbon monoxide (CO) 80.14 ppm	CG-0040-22	Nimt	14-Feb-27
Carbon monoxide (CO) 302 ppm	1915/23	Linde	16-Jan-25
Carbon monoxide (CO) 1003 ppm	2584/23	Linde	10-Sep-25
Nitrogen Dioxide (NO ₂) 30.34 ppm	2703/22	Linde	22-Aug-24
Nitrogen Dioxide (NO ₂) 81.32 ppm	3546/23	Linde	14-Jan-26
Nitrogen Dioxide (NO ₂) 201.9 ppm	1975/23	Linde	17-Jul-25
Nitric Oxide (NO) 30.01 ppm	CG-0014-23	Nimt	19-Feb-25
Nitric Oxide (NO) 151.5 ppm	0161/23	Linde	22-Jan-25
Nitric Oxide (NO) 322.5 ppm	1974/23	Linde	17-Jul-25
Sulphur Dioxide (SO ₂) 50.36 ppm	2004/23	Linde	17-Jul-25
Sulphur Dioxide (SO ₂) 100.8 ppm	3507/22	Linde	09-Nov-24
Sulphur Dioxide (SO ₂) 600.8 ppm	2003/23	Linde	17-Jul-25

Measured room conditions

Temperature : 23.5 °C Humidity : 64.1 %RH Pressure : 1011.7 mbar

Calibration conditions

Gas Temperature : 23 °C Flow rate : 1,200 ml/min Gas pressure : 1016.4 mbar

Calibration Results (Without adjustment) (Table 2)

Parameter of Standard	Standard Values	Mean of UUC	Error	Uncertainty (±)
O ₂ (%Vol)	2.50	2.57	0.07	0.15
O ₂ (%Vol)	10.04	10.09	0.05	0.20
O ₂ (%Vol)	21.02	21.08	0.06	0.30
CO (ppm)	80.14	81	0.86	3.0
CO (ppm)	302	302	0	6.0
CO (ppm)	1003	1002	-1	12
NO ₂ (ppm)	30.34	30.2	0.14	6.0
NO ₂ (ppm)	81.32	82.4	1.08	6.0
NO ₂ (ppm)	201.9	202.8	0.9	12
NO (ppm)	30.01	29	-1.01	6.0
NO (ppm)	151.5	150	-1.5	8.0
NO (ppm)	322.5	320	-2.5	12
SO ₂ (ppm)	50.36	49	-1.36	6.0
SO ₂ (ppm)	100.8	100	-0.8	6.0
SO ₂ (ppm)	600.8	599	-1.8	13

Remark : 1 cmol/mol = 1 %vol, 1 μmol/mol = 1 ppm.

End of Report

เอกสารไม่ควบคุม

CERTIFICATE OF CALIBRATION

Certificate No.: COF-032-67

Page 2 of 2 Pages

MEASUREMENT ITEM : Top Load Orifice
MANUFACTURER : Andersen Instruments
MODEL/TYPE : G25A
SERIAL NUMBER : 1301
ID NUMBER : UAE.ANY.051/2547
CONDITION AS-RECEIVED : Used item
CUSTOMER : United Analyst and Engineering Consultant Co., Ltd.
81 Soi Udomsuk 41, Sukhumvit Road, Bangkok, Phrakhanong,
Bangkok 10260

RECEIVED DATE : 04 Jul 2024
MEASUREMENT DATE : 16 Jul 2024
ISSUE DATE : 17 Jul 2024

ENVIRONMENTAL CONDITIONS:

Ambient condition in the laboratory are as follow:

Temperature : 23.0 ± 3.0 °C
Relative Humidity : 55.0 ± 5.0 %RH
Atmospheric Pressure : 1020 ± 10 hPa

CALIBRATION CONDITION:

Preconditioning : 24 hours at ambient conditions.

Measurement Condition : The average values during measurement are 23.9 °C and 53.0 %RH.

NOTED: The certificate is valid only to the item calibrated on date and place of calibration.

TABULATION OF RESULTS:

The table on next page give the measured values.

Calibration procedure:
The Orifice gas flow device was calibrated against
Standard Rotary Displacement Meter (Jirantees
Meter) Model G65/MC/M2-ep. The M2-C2-004
was used as a calibration guideline.

Traceability:
This certificate provides a traceability of the
measurement to realization of the national
standards used to realization of the International
system of units (SI) through the NIMT (National
Metrology Institute of Thailand) via Certificate
number: NIMT063-23.

Uncertainty of Measurement:
The reported uncertainty of measurement is based
on the standard uncertainty multiplied by a
coverage factor $k=2$, which for a normal
distribution corresponds to a coverage probability
of approximately 95%. The standard uncertainty
has been determined in accordance with the GUM
Evaluation of measurement data - Guide to the
expression of uncertainty in measurement.

MEASUREMENT RESULTS:

The Orifice gas flow device was calibrated by direct comparison method with the Standard Rotary Displacement Meter (Roots Meter). The humid air was used as a medium in the system. The standard conditions are 25°C (298.15 K) and 760 mmHg for standard temperature and standard pressure respectively.

Table 1: The results of Q Standard calibration data

Plate	Flow rate m ³ /min	Pressure [Pa] mmHg	Temperature [Ta] °C	Temperature [Tm] °C	Ap_meter mmHg	Ap_Office mmHg	F	Standard Flow [Qs] m ³ /min
1	0.704	757.245	23.88	22.89	56.199	1.651	1.285	0.654
2	1.004	757.257	23.90	22.96	62.578	3.293	1.115	0.924
3	1.115	757.425	24.24	23.58	41.738	4.308	2.075	1.055
4	1.167	757.384	24.38	23.68	31.029	4.932	2.319	1.121
5	1.413	757.295	24.44	23.83	29.757	7.230	2.687	1.358

Slope (m): 1.99535
Intercept (b): -0.02408
Correlation coefficient (r): 0.99977
Uncertainty (k=2): 0.015 m³/min

Table 2: The results of Q actual calibration data

Plate	Flow rate m ³ /min	Pressure [Pa] mmHg	Temperature [Ta] °C	Temperature [Tm] °C	Ap_meter mmHg	Ap_Office mmHg	F	Standard Flow [Qs] m ³ /min
1	0.704	757.245	23.88	22.89	56.199	1.651	0.805	0.854
2	1.004	757.257	23.90	22.96	62.578	3.293	1.137	0.924
3	1.115	757.425	24.24	23.58	41.738	4.908	1.301	1.056
4	1.167	757.384	24.38	23.68	31.029	4.932	1.302	1.122
5	1.413	757.295	24.44	23.83	29.757	7.230	1.686	1.361

Slope (m): 1.24874
Intercept (b): -0.01506
Correlation coefficient (r): 0.99977
Uncertainty (k=2): 0.015 m³/min

End of Certificate of Calibration

Calibrated by:
☐ Mr. Sengwit Thachetad
☒ Mr. Nitigorn Lertsomphol



Approved signatory: Mr. Parinya Booncharoen
Calibration Department Manager



THIS CERTIFICATE REPORT MAY NOT BE REPRODUCED EXCEPT IN FULL UNLESS PERMISSION FOR REPRODUCTION HAS BEEN OBTAINED
IN WRITING FROM THE LABORATORY

เอกสารไม่ควบคุม

เอกสารไม่ควบคุม



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG, BANGKOK 10250
TEL. 0-2717-3000-24 FAX. 0-2719-9484

Certificate of Calibration

Certificate No.: 24P1251
Page: 1 of 2

Equipment : U Tube Manometer
Manufacturer : Dwyer
Model : 1221-36-W/M
Serial No. : -
ID No. : UAE.EFM.077/2566

Condition As-Received: Used Item

Received Date: 03 April 2024

Calibration Date: 11 April 2024

Reference: 2404-0118WSC Submitted by: United Analyst and Engineering Consultant Co., Ltd.

Ambient Temperature: (23 ± 2) °C

Relative Humidity: (50 ± 15) %

Atmospheric Pressure: 1012 mbar

Procedure used: The calibration was conducted by direct comparison method against Pressure Measuring Instruments
Standard according to calibration procedure CP-P04, using "DKD-R 6-1 ; Calibration of Pressure Gauges " as a guidelines.

Condition of this result of calibration

1.Reference standards instruments :

Instrument	Model	Serial No.	Certificate No.	Due Date
1) Pressure Calibrator	PC106P	1189	MP-0176-23	12 Sep 2024

2.This result of calibration was made on requested at the point specified by customer.

3.Scale and conversion factor is 1 kPa = 4.0146293 inH₂O

4.This instrument was used clean air as pressure media.

5.This instrument was calibrated by applied pressure to high-port (+) side and low-port (-) side open to atmospheric pressure.

6.This instrument was installed in vertical orientation and top of the pressure port was used as the reference level.

7.The certificate is valid only to the item calibrated on date and place of calibration.

8.This Certification is traceable to the International System of Unit maintained through:-

-National Institute of Metrology (Thailand), NSC-ONSC Accredited No. Calibration 0144



Cert.No.: 24P1251
Page: 2 of 2

Result of calibration:- Without adjustment

Function:- Pressure Measurement

Increasing Pressure

Range : 0 inH₂O to 36 inH₂O

Scale Interval : 0.1 inH₂O (The Second Estimate)

Applied Pressure	High-port side	UUC Indication Low-port side	ΔP	Error
0.00	0.00	0.00	0.00	0.00
2.00	1.00	-1.00	2.00	0.00
4.00	2.00	-2.00	4.00	0.00
6.00	3.00	-3.00	6.00	0.00
8.00	4.00	-4.00	8.00	0.00
10.00	5.00	-5.00	10.00	0.00
12.00	6.00	-6.00	12.00	0.00
14.00	7.05	-7.05	14.10	0.10
16.00	8.05	-8.05	16.10	0.10
18.00	9.05	-9.05	18.10	0.10
20.00	10.05	-10.05	20.10	0.10
22.00	11.05	-11.05	22.10	0.10
24.00	12.05	-12.05	24.10	0.10
26.00	13.05	-13.05	26.10	0.10
28.00	14.05	-14.05	28.10	0.10
30.00	15.05	-15.05	30.10	0.10
32.00	16.05	-16.10	32.15	0.15
34.00	17.05	-17.10	34.15	0.15
35.80	18.00	-18.00	36.00	0.20

The uncertainty of measurement was ± 0.11 inH₂O

* ΔP = High-port side - Low-port side

* UUC = Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k=2$, providing a level of confidence of approximately 95 %.

-000-

Calibrated by : Suksan Khankaew
Issue Date : 17 April 2024

Approved Signatory :
[] Phalinee Prabpaipal
[] Sura Suwanmasri
[✓] Attapol Panurach

เอกสารไม่ควบคุม

เอกสารไม่ควบคุม



Certificate of Calibration

Certificate No. : 24P1369
Page : 1 of 2

Equipment : Aneroid Barometer
Manufacturer: Barigo
Model : -
Serial No.: -
ID No.: UAE,ANV,013/2547

Condition As-Received: Used Item
Received Date: 05 April 2024
Calibration Date: 22 April 2024

Reference: 2404-0243WSC
Ambient Temperature: (23 ± 2) °C
Relative Humidity: (50 ± 15) %
Atmospheric Pressure: 1007 mbar
Submitted by: United Analyst and Engineering Consultant Co.,Ltd.
81 Soi Udumsuk 41, Sukhumvit Road, Bangchak,
Phrakhanong, Bangkok 10260

Procedure used: The calibration was conducted by direct comparison method against Pressure Measuring Instruments Standard according to calibration procedure CP-P10, using " DKD-R 6-1 ; Calibration of Pressure Gauges " as a guidelines.

Condition of this result of calibration

1.Reference standards instruments :

Instrument	Model	Serial No.	Certificate No.	Due Date
1) Standard Barometer	DPI142	1422505046	MP-0094-23	03 May 2024

2.This instrument was installed in vertical orientation and center of the dial was used as the reference level.

3.This result of calibration was made on requested at the point specified by customer.

4.Scale and conversion factor is 1 kPa = 7.50062 mmHg

5.This result of calibration instrument was in absolute pressure.

6.This instrument was used clean air as pressure media.

7.The certificate is valid only to the item calibrated on date and place of calibration.

8.This Certification is traceable to the International System of Unit maintained through-

-National Institute of Metrology Thailand (NIMT)

Calibrated by : Suksan Khankaew
Issue Date : 23 April 2024

Approved Signatory :
[] Phalinee Prabpaijal
[] Sura Suwannasri
[✓] Attapol Panurach

เอกสารไม่ควบคุม



Cert.No.: 24P1369
Page: 2 of 2

Result of calibration:- Without adjustment

Function:- Absolute Pressure Measurement

Range : 720 mmHg to 780 mmHg

Scale Interval : 1 mmHg (The Fifth Estimate)

Increasing Pressure

Applied Pressure (mmHg)	718,40	729,71	740,61	751,07	761,97	773,05	786,91
UUC* Indication (mmHg)	720,0	730,0	740,0	750,0	760,0	770,0	780,0
Error (mmHg)	1,60	0,29	-0,61	-1,07	-1,97	-3,05	-6,91

Decreasing Pressure

Applied Pressure (mmHg)	786,91	772,99	761,71	750,69	740,13	729,35	718,44
UUC* Indication (mmHg)	780,0	770,0	760,0	750,0	740,0	730,0	720,0
Error (mmHg)	-6,91	-2,99	-1,71	-0,69	-0,13	0,65	1,56

The uncertainty of measurement was ± 0,24 mmHg

* UUC = Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95 %.

-000-

เอกสารไม่ควบคุม



Certificate of Calibration

Certificate No. : 24H753
Page : 1 of 2

Equipment : Dial Thermo-Hygrometer
Manufacturer: Barigo
Model : -
Serial No.: -
ID No.: UAE,ANV,127/2550

Condition As-Received: Used Item
Received Date: 05 April 2024
Calibration Date: 10 April 2024
to 18 April 2024

Reference: 2404-0247WSC
Ambient Temperature: (25 ± 3) °C
Relative Humidity: (50 ± 20) %
Submitted by: United Analyst and Engineering Consultant Co.,Ltd.
81 Soi Udumsuk 41, Sukhumvit Road,
Bangchak, Phrakhanong, Bangkok 10260

Procedure used: Calibration were conducted using in-house calibration procedure CP-H02 according to comparison with standard chilled mirror sensor for humidity measurement function and comparison with standard temperature probe for temperature measurement function into humidity / temperature chamber.

Condition of this result of calibration

1.Reference standards instruments :

Instrument	Model	Serial No.	Certificate No.	Due Date
1) Chilled Mirror Hygrometer	Dew Master	44730	21656	02 Aug 2024
2) Handheld Thermometer With Sensor	1521	A5A339	231238	16 Oct 2024

2.The certificate is valid only to the item calibrated on date and place of calibration.

3.This Certification is traceable to the International System of Unit maintained through-

-Thunder Scientific Corporation, NVLAB Accreditation No. Calibration 200582-0

-Technology Promotion Association (Thailand-Japan), NSC-ONSC Accredited No. Calibration 0008

Calibrated by : Chakrit Waewwanjua
Issue Date : 18 April 2024

Approved Signatory :
[] Chakrit Waewwanjua
[✓] Vipom Tantiyawutti
[] Unnopphol Harachai

เอกสารไม่ควบคุม



Cert. No.: 24H753
Page: 2 of 2

Result of Calibration:-

Function: Humidity Measurement.

Without Adjustment

Reference Temperature (°C)	Standard Humidity (%R.H.)	UUC* Reading (%R.H.)	Error (%R.H.)	Uncertainty of Measurement (±%R.H.)
25,0	40,1	43	2,9	1,6
25,0	60,0	60	0,0	1,7
25,0	80,0	78	-2,0	1,8

Result of Calibration:-

Function: Temperature Measurement.

Without Adjustment

Standard Temperature (°C)	UUC* Reading (°C)	Error (°C)	Uncertainty of Measurement (±°C)
20,014	20,0	-0,014	0,72
25,033	25,0	-0,033	0,72
30,010	30,0	-0,010	0,72
35,027	34,5	-0,527	0,72
40,013	39,5	-0,513	0,72

UUC* : Unit Under Calibration

The reported uncertainty of measurement was base on standard uncertainty multiplied by coverage factor $k = 2,00$, providing confidence level approximately 95%.

-000-

เอกสารไม่ควบคุม

MULTI-POINT GAS TEST REPORT


Test Date : Sep 17, 2024

Equipment : Gas Analyzer (NO₂) Model : 42i
Manufacturer : Thermo Scientific Serial Number : CM08130002

Standard Gas Concentration		Dilutor Detail	
Sulphur Dioxide (SO ₂)	42.89 PPM	Manufacturer :	Thermo Scientific
Nitric Oxide (NO)	46.77 PPM	Model :	146i
Methane (CH ₄)	- PPM	Serial Number :	1180540071
Carbon Monoxide (CO)	965.9		
Cylinder No. :	EB0159156		
Expiration Date :	Nov 6, 2026		

Multi-point gas test data

Reference Value (ppb)		Analyzer Display (ppb)	Difference Error	Percent Error	[% Error]
Level 1	Zero	0.0	0.5	0.50	0.50
Level 2	20.00%	100.0	101.6	1.60	1.57
Level 3	40.00%	200.0	200.5	0.50	0.25
Level 4	60.00%	300.0	300.8	0.80	0.27
Level 5	80.00%	400.0	400.0	0.00	0.00
Remark : Measuring Range		500.0 ppb	Average Difference (%)		0.52

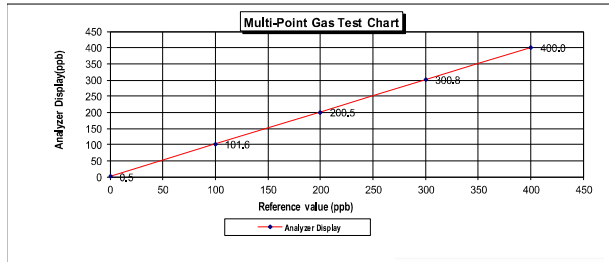

Calculate by
17/9/2567

Approve by
17 Sep 2024

MULTI-POINT GAS TEST REPORT


Test Date : Sep 20, 2024

Equipment : Gas Analyzer (NO₂) Model : 42i
Manufacturer : Thermo Scientific Serial Number : CM19050148

Standard Gas Concentration		Dilutor Detail	
Sulphur Dioxide (SO ₂)	42.89 PPM	Manufacturer :	Thermo Scientific
Nitric Oxide (NO)	46.77 PPM	Model :	146i
Methane (CH ₄)	- PPM	Serial Number :	1180540071
Carbon Monoxide (CO)	965.9		
Cylinder No. :	EB0159156		
Expiration Date :	Nov 6, 2026		

Multi-point gas test data

Reference Value (ppb)			Analyzer Display (ppb)	Difference Error	Percent Error	[% Error]	
Level 1	Zero	0.0	0.0	0.00	0.00	0.00	
Level 2	20.00%	100.0	100.7	0.70	0.70	0.70	
Level 3	40.00%	200.0	200.6	0.60	0.30	0.30	
Level 4	60.00%	300.0	300.9	0.90	0.30	0.30	
Level 5	80.00%	400.0	400.0	0.00	0.00	0.00	
Remark : Measuring Range			500.0 ppb		Average Difference (%)		0.26

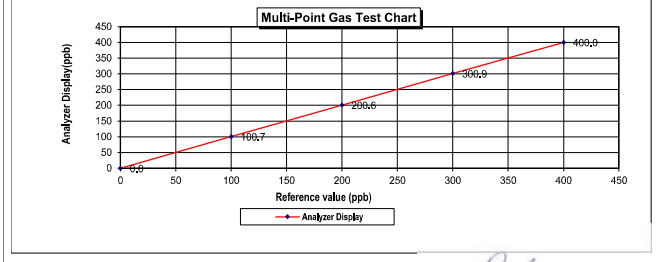

Calculate by
20/9/2567

Approve by
20 Sep 2024

MULTI-POINT GAS TEST REPORT


Test Date : Sep 17, 2024

Equipment : Gas Analyzer (NO₂) Model : 42i
Manufacturer : Thermo Scientific Serial Number : CM19050149

Standard Gas Concentration		Dilutor Detail	
Sulphur Dioxide (SO ₂)	42.89 PPM	Manufacturer :	Thermo Scientific
Nitric Oxide (NO)	46.77 PPM	Model :	146i
Methane (CH ₄)	- PPM	Serial Number :	1180540071
Carbon Monoxide (CO)	965.9		
Cylinder No. :	EB0159156		
Expiration Date :	Nov 06, 2026		

Multi-point gas test data

Reference Value (ppb)			Analyzer Display (ppb)	Difference Error	Percent Error	[% Error]
Level 1	Zero	0.0	0.0	0.00	0.00	0.00
Level 2	20.00%	100.0	100.8	0.80	0.79	0.79
Level 3	40.00%	200.0	200.6	0.60	0.30	0.30
Level 4	60.00%	300.0	300.7	0.70	0.23	0.23
Level 5	80.00%	400.0	400.0	0.00	0.00	0.00
Remark : Measuring Range			500.0 ppb	Average Difference (%)		0.27

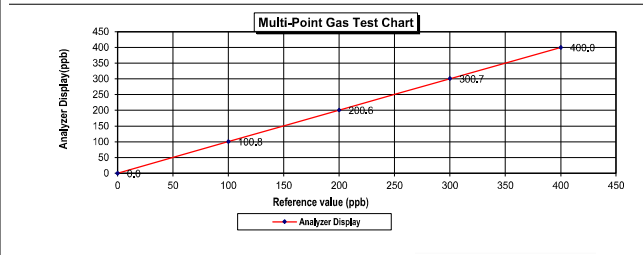

Calculate by
17/9/2567

Approve by
17 Sep 2024

CERTIFICATE OF ANALYSIS

Grade of Product: EPA PROTOCOL STANDARD

Customer: AIR LIQUIDE (THAILAND)
LTD -
Part Number: E05N191E15A0014
Cylinder Number: E0162121
Laboratory: 124 - Plumsteadville - PA
PGVP Number: A12023
Gas Code: CO, CO₂, NO, NO₂, SO₂, BALN
Reference Number: 180-402772205-1
Cylinder Volume: 144.0 CF
Cylinder Pressure: 2016 PSIG
Valve Outlet: 650
Certification Date: Jul 06, 2023
Expiration Date: Jul 06, 2031

Certification performed in accordance with EPA Traceability Protocol for Assay and Certification of Gasware Calibration Standards (May 2012) document EPA 800/R-12/031, using the assay procedures listed. Analytical Methodology does not require correction for analytical interference. This cylinder has a total analytical uncertainty as stated below with a confidence level of 95%. There are no significant impurities which affect the use of this calibration mixture. All concentrations are of a midrange basis unless otherwise noted. The results were only in the units listed. The report shall not be reproduced except in full without approval of the laboratory. Do Not Use This Cylinder below 100 psig, i.e. 0.7 megapascals.

ANALYTICAL RESULTS					
Component	Requested Concentration	Actual Concentration	Protocol Method	Total Relative Uncertainty	Assay Dates
NOX	100.0 PPM	100.4 PPM	G1	$\pm 0.9\%$ NIST Traceable	06/27/2023, 07/06/2023
NITRIC OXIDE	100.0 PPM	100.2 PPM	G1	$\pm 0.9\%$ NIST Traceable	06/27/2023, 07/06/2023
SULFUR DIOXIDE	100.0 PPM	100.0 PPM	G1	$\pm 1.4\%$ NIST Traceable	06/27/2023, 07/06/2023
CARBON MONOXIDE	200.0 PPM	200.0 PPM	G1	$\pm 0.3\%$ NIST Traceable	06/26/2023
CARBON DIOXIDE	8,000 %	7,982 %	G1	$\pm 1.2\%$ NIST Traceable	06/27/2023
NITROGEN	Balance				
CALIBRATION STANDARDS					
Type	Lot ID	Cylinder No	Concentration	Uncertainty	Expiration Date
GMIS	104202308	CC754364	98.36 PPM NITRIC OXIDE/NITROGEN	$\pm 0.4\%$	Jan 04, 2031
PRM	C2219101	AP61514048	100.15 PPM NITRIC OXIDE/NITROGEN	$\pm 0.3\%$	Feb 28, 2025
GMIS	2023042525	CC754381	98.52 PPM NITRIC OXIDE/NITROGEN	$\pm 0.4\%$	Apr 25, 2031
PRM	12409	D913660	15.01 PPM NITROGEN DIOXIDE/AIR	$\pm 1.5\%$	Feb 17, 2023
GMIS	153400202002	EB0130037	9.893 PPM NITROGEN DIOXIDE/NITROGEN	$\pm 1.6\%$	Sep 29, 2025
NTRM	160102-22	KAL803829	97.69 PPM SULFUR DIOXIDE/NITROGEN	$\pm 0.8\%$	Nov 01, 2027
CO	230601	CC745902	249.47 PPM CARBON MONOXIDE/NITROGEN	$\pm 0.3\%$	Dec 09, 2028
NTRM	130805-02	CC411730	13.359 % CARBON DIOXIDE/NITROGEN	$\pm 0.6\%$	May 14, 2025
The SRM, NTRM, PRM, or RGM noted above is only in reference to the GMS used in the assay and not part of the analysis.					
ANALYTICAL EQUIPMENT					
Instrument/Make/Model	Analytical Principle		Last Multipoint Calibration		
Nicolet iS50 FTIR AUP2010245 CO ₂	FTIR		Jun 15, 2023		
SIEMENS ULTRAMATE6 N1-C8-180	NDIR		Jun 14, 2023		
Nicolet iS50 FTIR AUP2010245 NO	FTIR		Jun 29, 2023		
Nicolet iS50 FTIR AUP2010245 NO ₂	FTIR		Jun 15, 2023		
Nicolet iS50 FTIR AUP2010245 SO ₂	FTIR		Jun 08, 2023		

Approved for Release

MULTI-POINT GAS TEST REPORT


Test Date : Sep 6, 2024

Equipment : Gas Analyzer (SO₂) Model : 43i
Manufacturer : Thermo SCIENTIFIC Serial Number : CM22387061

Standard Gas Concentration			Dilutor Detail	
Sulphur Dioxide (SO ₂)	42.89	PPM	Manufacturer :	Thermo SCIENTIFIC
Nitric Oxide (NO)	46.77	PPM	Model :	146i
Methane (CH ₄)	-	PPM	Serial Number :	1180540071
Carbon Monoxide (CO)	965.9			
Cylinder No. :	EB0159156			
Expiration Date :	Nov 06, 2026			

Multi-point gas test data

Reference Value (ppb)			Analyzer Display (ppb)	Difference Error	Percent Error	[% Error]
Level 1	Zero	0.0	0.0	0.00	0.00	0.00
Level 2	20.00%	100.0	100.7	0.70	0.70	0.70
Level 3	40.00%	200.0	200.7	0.70	0.35	0.35
Level 4	60.00%	300.0	301.1	1.10	0.37	0.37
Level 5	80.00%	400.0	400.0	0.00	0.00	0.00
Remark : Measuring Range		500.0 ppb		Average Difference (%)		0.28

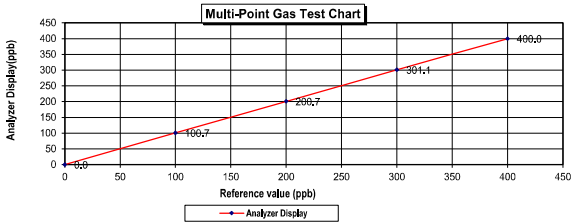

Calculate by
Gichai C.
6 / 9 / 2567

Approve by
Ratan K.
6 / Sep / 2024

MULTI-POINT GAS TEST REPORT


Test Date : June 19, 2024

Equipment : Gas Analyzer (SO₂) Model : 43i
Manufacturer : Thermo SCIENTIFIC Serial Number : CM22387063

Standard Gas Concentration			Dilutor Detail	
Sulphur Dioxide (SO ₂)	42.89	PPM	Manufacturer :	Thermo SCIENTIFIC
Nitric Oxide (NO)	46.77	PPM	Model :	146i
Methane (CH ₄)	-	PPM	Serial Number :	1180540071
Carbon Monoxide (CO)	965.9			
Cylinder No. :	EB0159156			
Expiration Date :	Nov 06, 2026			

Multi-point gas test data

Reference Value (ppb)			Analyzer Display (ppb)	Difference Error	Percent Error	[% Error]
Level 1	Zero	0.0	0.0	0.00	0.00	0.00
Level 2	20.00%	100.0	100.8	0.80	0.79	0.79
Level 3	40.00%	200.0	200.7	0.70	0.35	0.35
Level 4	60.00%	300.0	301.1	1.10	0.37	0.37
Level 5	80.00%	400.0	400.0	0.00	0.00	0.00
Remark : Measuring Range			500.0 ppb	Average Difference (%)		0.30

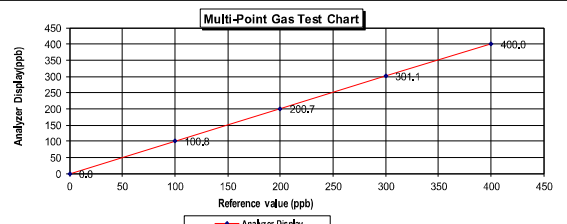

Calculate by
Gichai C.
19 / 06 / 2567

Approve by
Ratan K.
19 / June / 2024

MULTI-POINT GAS TEST REPORT


Test Date : May 15, 2024

Equipment : Gas Analyzer (SO₂) Model : 43i
Manufacturer : Thermo SCIENTIFIC Serial Number : CM22387067

Standard Gas Concentration			Dilutor Detail	
Sulphur Dioxide (SO ₂)	44.68	PPM	Manufacturer :	Thermo SCIENTIFIC
Nitric Oxide (NO)	45.94	PPM	Model :	146i
Methane (CH ₄)	-	PPM	Serial Number :	1180540071
Carbon Monoxide (CO)	984.8			
Cylinder No. :	EB0143262			
Expiration Date :	Jun 24, 2024			

Multi-point gas test data

Reference Value (ppb)			Analyzer Display (ppb)	Difference Error	Percent Error	[% Error]
Level 1	Zero	0.0	0.9	0.90	0.90	0.90
Level 2	20.00%	100.0	100.8	0.80	0.79	0.79
Level 3	40.00%	200.0	200.9	0.90	0.45	0.45
Level 4	60.00%	300.0	300.9	0.90	0.30	0.30
Level 5	80.00%	400.0	400.0	0.00	0.00	0.00
Remark : Measuring Range		500.0 ppb		Average Difference (%)		0.49

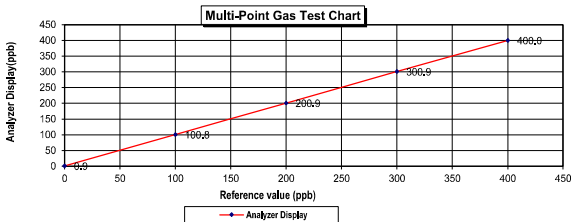

Calculate by
Gichai C.
15 / 05 / 2567

Approve by
Ratan K.
15 / May / 2024

CERTIFICATE OF ANALYSIS Grade of Product: EPA PROTOCOL STANDARD

Customer: AIR LIQUIDE (THAILAND)
LTD.
Part Number: E05N191E15A0014
Cylinder Number: EB0162121
Laboratory: 124 - Plumsteadville - PA
PGVP Number: A12023
Gas Code: CO, CO₂, NO, NO₂, SO₂, BALN
Reference Number: 180-402772205-1
Cylinder Volume: 144.0 CF
Cylinder Pressure: 2016 PSIG
Valve Outlet: 650
Certification Date: Jul 06, 2023
Expiration Date: Jul 06, 2031

Certification performed in accordance with "EPA Traceability Protocol for Assay and Certification of Gasware Calibration Standards (May 2012)" document EPA 800/R-12/031, using the assay procedures listed. Analytical Methodology does not require correction for analytical interference. This cylinder has a total analytical uncertainty as stated below with a confidence level of 95%. There are no significant impurities which affect the use of this calibration mixture. All concentrations are of a midrange basis unless otherwise noted. The results were only in the form listed. The report shall not be reproduced except in full without approval of the laboratory. Do Not Use This Cylinder below 100 psig, i.e. 0.7 megapascals.

ANALYTICAL RESULTS					
Component	Requested Concentration	Actual Concentration	Protocol Method	Total Relative Uncertainty	Assay Dates
NOX	100.0 PPM	100.4 PPM	G1	\pm 0.9% NIST Traceable	06/27/2023, 07/06/2023
NITRIC OXIDE	100.0 PPM	100.2 PPM	G1	\pm 0.9% NIST Traceable	06/27/2023, 07/06/2023
SULFUR DIOXIDE	100.0 PPM	100.0 PPM	G1	\pm 1.4% NIST Traceable	06/27/2023, 07/06/2023
CARBON MONOXIDE	200.0 PPM	199.2 PPM	G1	\pm 0.3% NIST Traceable	06/26/2023
CARBON DIOXIDE	8,000 %	7,982 %	G1	\pm 1.2% NIST Traceable	06/27/2023
NITROGEN	Balance				
CALIBRATION STANDARDS					
Type	Lot ID	Cylinder No	Concentration	Uncertainty	Expiration Date
GMIS	104202308	CC754364	98.36 PPM NITRIC OXIDE/NITROGEN	\pm 0.4%	Jan 04, 2031
PRM	C2219101	AP1514048	100.15 PPM NITRIC OXIDE/NITROGEN	\pm 0.3%	Feb 28, 2025
GMIS	2023042525	CC754381	98.52 PPM NITRIC OXIDE/NITROGEN	\pm 0.4%	Apr 25, 2031
PRM	12409	D913660	15.01 PPM NITROGEN DIOXIDE/AIR	\pm 1.5%	Feb 17, 2023
GMIS	153400202002	EB0130037	9.893 PPM NITROGEN DIOXIDE/NITROGEN	\pm 1.6%	Sep 29, 2025
NTRM	160102-22	KAL803829	97.69 PPM SULFUR DIOXIDE/NITROGEN	\pm 0.8%	Nov 01, 2027
CO	230601	CC745902	249.47 PPM CARBON MONOXIDE/NITROGEN	\pm 0.3%	Dec 09, 2028
NTRM	130806-02	CC411739	13.359 % CARBON DIOXIDE/NITROGEN	\pm 0.6%	May 14, 2025
The SRM, NTRM, PRM, or RGM noted above is only in reference to the GMS used in the assay and not part of the analysis.					
ANALYTICAL EQUIPMENT					
Instrument/Make/Model	Analytical Principle		Last Multipoint Calibration		
Nicolet iS50 FTIR AUP2010245 CO ₂	FTIR		Jun 15, 2023		
SIEMENS ULTRAMATE6 N1-C8-180	NDIR		Jun 14, 2023		
Nicolet iS50 FTIR AUP2010245 NO	FTIR		Jun 29, 2023		
Nicolet iS50 FTIR AUP2010245 NO ₂	FTIR		Jun 15, 2023		
Nicolet iS50 FTIR AUP2010245 SO ₂	FTIR		Jun 08, 2023		

Approved for Release

Certificate of Calibration

Customer

Name : UNITED ANALYST AND ENGINEERING
CONSULTANT CO.,LTD.
Address : 81 Soi Udomsuk 41, Sukhumvit Road, Bangchak,
Prakanong, Bangkok 10260

Certificate No : 24-ACT-091
Request No : Req-2024-1380

Unit Under Calibration Details

Measurement item : Acoustic Calibrator
Manufacturer : SVANTEK
Model : SV 36
Serial Number : 107224
ID : UAE.EFM.171/2564
Class : 1
Range : 94 , 114 dB / 1000 Hz
Instrument Status : Used

Calibration Environment and Details


Temperature : (23 ±2 °C)
Humidity : (50 ± 20 %RH)
Barometric Pressure : (1013 ±10.0 hPa)
Received Date : 24 June 2024
Calibration Date : 26 June 2024
Location of Calibration : LAB 1 Acoustic
Calibration Procedure : In-house method CP-ACT-02 based on IEC 60942:2017 Electroacoustics - Sound calibrators


Reference Standard	Model	Serial Number	Traceable	Due Calibration
Sound Calibrator	SV 35A	58079	EEI	12 June 2025
THD Multimeter	2015	1047765	NIMT	16 January 2025

Traceability : This certificate provides traceability of measurement to recognized national standard, and to the realization of the international System of Units (SI).

Note

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor $k=2$, providing a level of confidence approximately 95 %.

Calibrated By : 
Mr. Noppadon Luangart
Service Calibration Engineer

Approved By : 
Mr. Pacit Mathavorn
Calibration Engineer Supervisor

Issue Date : 26 June 2024

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Issuing Laboratory.
FIM-708-ACT-02 Rev.03 Issue date 5/6/24

เอกสารไม่ควบคุม

Certificate No : 24-ACT-091

Request No : Req-2024-1380

Sound pressure level

Calibration Results : Without Adjustment

Calibration Range (dB)	Without Adjustment (dB)		Adjustment (dB)		Uncertainty (± dB)	Acceptance limit Class 1 (± dB)	Result
	Measured	Deviated value	Measured	Deviated value			
94 dB / 1000 Hz	94.02	0.02	-	-	0.14	0.25	Pass
114 dB / 1000 Hz	114.05	0.05	-	-	0.13	0.25	Pass

Frequency of Sound pressure level

Calibration Range (Hz)	Without Adjustment		Adjustment		Uncertainty (± %)	Acceptance limit Class 1 (± %)	Result
	Measured (Hz)	Deviated	Measured (Hz)	Deviated			
94 dB / 1000 Hz	1000.00	0.00	-	-	0.01	0.70	Pass
114 dB / 1000 Hz	1000.00	0.00	-	-	0.01	0.70	Pass

Total Harmonic Distortion plus Noise of Sound pressure level (THD+N %)

Calibration Range (Hz)	Without Adjustment	Adjustment	Uncertainty (± %)	Acceptance limit	Result
	Measured (%)	Measured (%)			
94 dB / 1000 Hz	0.24	-	0.40	2.5	Pass
114 dB / 1000 Hz	0.44	-	0.40	2.5	Pass

Note :

Function	Maximum-permitted Uncertainty of measurement
Sound pressure level	0.15 dB
Frequency	0.20%
Total distortion+noise	0.50%

- Acceptance limit was IEC60942:2017 Class 1
- The calibration results exclude the calibration pressure correction
- The calibration results exclude the microphone volume correction

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Issuing Laboratory.
FIM-708-ACT-02 Rev.03 Issue date 5/6/24

เอกสารไม่ควบคุม

Certificate No : 24-ACT-091

Request No : Req-2024-1380

Decision Rule for Statements of Conformity


The standard decision rule employed for the statements of conformity to each calibration result will be applied using ILAC-G8:09/2019: Guidelines on the Reporting of Compliance with Specification as following Fig and statements

Pass : The measurement result plus the expanded uncertainty with a 95% coverage probability were within the limit.

Pass^B : The measurement result was within the limit. However, a portion of the expanded uncertainty of measurement at 95% exceeds the limit.

Fail^B : The measurement result was out of the limit. However, a portion of the expanded uncertainty of measurement at 95% is within the limit.

Fail : The measurement result plus the expanded uncertainty with a 95% coverage probability were outside the limit.

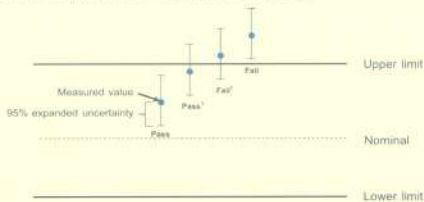

End of Calibration

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Issuing Laboratory.
FIM-708-ACT-02 Rev.03 Issue date 5/6/24

เอกสารไม่ควบคุม



ELECTRICAL AND ELECTRONICS INSTITUTE
FOUNDATION FOR INDUSTRIAL DEVELOPMENT

975 Moo 4, Bangpoo Industrial Estate, Soi 8, Sukhumvit Road km 37,
Phraek Sa, Mueang Samut Prakan, Samut Prakan 10280
Tel : +66 2709 4860 Fax: +66 2324 0917



Certificate No.: CP20240292EA
Operation No.: CP2024070255

Certificate of Calibration

Equipment: Sound Level Meter
Manufacturer: Larson Davis (Meter), PCB (Microphone), PCB (Preamplifier)
Model/Type: LxT2 (Meter), 375B02 (Microphone), PRLxT2B (Preamplifier)
Serial No.: 0005348 (Meter), 11800 (Microphone), 056140 (Preamplifier)
ID No.: UAE.EFM.045/2563
Customer: United Analyst and Engineering Consultant Co.,Ltd.
Address: 81 Soi Udomsuk 41, Sukhumvit Road, Bangchak
Phrakhanong, Bangkok 10260
Received Date: 25 July 2024
Calibrated Date: 6 - 7 August 2024
Issued Date: 7 August 2024
Calibrated by: Ms. Juntaporn Kunhakom

Approved by: 
(Mr. Sittichai Swaksuriyawong)
Group Manager

This report was prepared electronically using applicable electronic signature. Printing or copy of file are considered as a copy of the document.
The reported uncertainty of measurement was based on standard uncertainty multiplied by a coverage factor (k) providing a level of confidence of approximately 95%. This certificate may not be reproduced other than in full except with the prior written approval of the Electrical and Electronics Institute, Foundation for Industrial Development.

เอกสารไม่ควบคุม

Certificate No.: CP20240292EA

Calibration Report

Equipment: Sound Level Meter
Manufacturer: Larson Davis (Meter), PCB (Microphone), PCB (Preamplifier)
Model/Type: LxT2 (Meter), 375B02 (Microphone), PRMLxT2B (Preamplifier)
Serial No.: 0005348 (Meter), 11800 (Microphone), 056140 (Preamplifier)
ID No.: UAE EFM.045/2563
Ambient Temperature: (23 ± 2) °C
Relative Humidity: (50 ± 15) %
Pressure: (101.3 ± 1.5) kPa

Method of Calibration :-
IEC 61672-3:2013.

Condition of this result of calibration

1. Reference standards instrument :-

	Instrument	Model	Serial No.	Cert. No.	Due Date
1)	Standard microphone	4180	2787490	AA-1012-23	12 November 2024
2)	Arbitrary Function Generator	AFG2021	C010063	CK20240048EA	23 June 2025
3)	Programmable Attenuator	PA5	2755	EF-0040-23	1 October 2024
4)	6.5 Digit precision multimeter	8846A	9610014	CB20230200EA	15 November 2024
5)	Pressure humidity and Temperature Transmitter	PTU301	L3950483	CL1-P240023 CD20240142EA	24 March 2025 12 June 2025
6)	Pressure humidity and Temperature Transmitter	PTU301	L3950484	CL1-P240030 CD20240143EA	11 April 2025 12 June 2025
7)	Performance Audio Analyzer	U8903B	MY56510003	CB20240035EB CK20230072EA	13 February 2025 13 September 2024

2. This result of calibration was found accurate as shown on date and place of calibration only.

3. This certification is traceable to the international system of unit maintained at :-

Reference standards instrument for Acoustic function

- National Institute of Metrology (Thailand)

Reference standards instrument for Electrical function

- National Institute of Metrology (Thailand)

- Electrical and Electronics Institute; NSC Accredited Calibration No.0119

Result of Calibration:-

Function : 1. Indication at the calibration check frequency

Reference Acoustic Signal (dB)	Measured value (dB)	Deviation (dB)	Acceptance limits (dB)
-	-	-	-

เอกสารไม่ควบคุม

Page 2 of 6

F-CAL-005 Ed.1

Certificate No.: CP20240292EA

Calibration Report

5.2 Time weighting at 1 kHz

Time Weighting	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
Fast	94.0	0.0	±0.1
Slow	94.0	0.0	±0.1
LAeq	94.0	0.0	±0.1

Function : 6. Long-Term Stability

Long-term stability over 30 minutes, with steady 1 kHz signal at reference level.

Time Period to Apply Signal (min)	Reference SPL (dB)	Record SPL at Conclusion of Time Period (dB)	Deviated value (dB)	Acceptance limits (dB)
30	94.0	94.0	0.0	±0.3

Function : 7. Level Linearity on the reference level range

7.1 Level Linearity on the reference level range, Upper

Anticipated Value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
94.0	94.0	0.0	±1.1
99.0	99.0	0.0	±1.1
104.0	104.0	0.0	±1.1
109.0	109.0	0.0	±1.1
114.0	114.0	0.0	±1.1
119.0	119.0	0.0	±1.1
124.0	124.0	0.0	±1.1
129.0	129.0	0.0	±1.1
134.0	134.1	0.1	±1.1
139.0	139.1	0.1	±1.1
140.0	140.1	0.1	±1.1
141.0	141.1	0.1	±1.1
142.0	142.1	0.1	±1.1

เอกสารไม่ควบคุม

Page 4 of 6

F-CAL-005 Ed.1

Certificate No.: CP20240292EA

Calibration Report

Function : 2. Self-generated Noise

2.1 Microphone Installed

Measured value (dB)
31.6

2.2 Microphone replaced by the electrical input signal device

Frequency Weighting	Measured value (dB)
A-weighting	31.5
C-weighting	31.6
Z-weighting	36.6

Function : 3. Acoustical signal tests of frequency weightings (Without Windscreen)

Meter free-field acoustic response at a level of 84 dB.

Frequency (Hz)	Deviation from various Frequency Weighting Response Curve			
	C-Weighting (dB)	A-Weighting (dB)	Z-Weighting (dB)	Acceptance limits (dB)
125	0.3	0.2	0.2	±1.5
1000	-0.2	-0.2	-0.2	±1.0
8000	2.9	2.9	2.9	±5.0

Function : 4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various Frequency Weighting Response Curve			
	C-Weighting (dB)	A-Weighting (dB)	Z-Weighting (dB)	Acceptance limits (dB)
63	0.0	0.0	0.0	±2.0
125	0.0	0.0	0.0	±1.5
250	0.0	0.0	0.0	±1.5
500	0.1	0.0	0.0	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.1	0.0	0.0	±2.0
4000	0.0	0.0	0.0	±3.0
8000	0.0	0.0	0.1	±5.0

Function : 5. Frequency and time weighting at 1 kHz

5.1 Frequency weighting at 1 kHz

Frequency Weighting	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
C-weighting	94.0	0.0	±0.2
A-weighting	94.0	0.0	±0.2
Z-weighting	94.0	0.0	±0.2

เอกสารไม่ควบคุม

Page 3 of 6

F-CAL-005 Ed.1

Certificate No.: CP20240292EA

Calibration Report

7.2 Level Linearity on the reference level range, Lower

Anticipated Value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
94.0	94.0	0.0	±1.1
89.0	89.0	0.0	±1.1
84.0	84.0	0.0	±1.1
79.0	79.0	0.0	±1.1
74.0	74.0	0.0	±1.1
69.0	69.0	0.0	±1.1
64.0	64.0	0.0	±1.1
59.0	59.0	0.0	±1.1
54.0	54.0	0.0	±1.1
49.0	49.0	0.0	±1.1
44.0	44.1	0.1	±1.1
43.0	43.2	0.2	±1.1
42.0	42.3	0.3	±1.1
41.0	41.4	0.4	±1.1
40.0	40.5	0.5	±1.1

Function : 8. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
Fast	200	136.0	0.0	±1.0
	2	118.8	-0.2	+1.0 ; -2.5
	0.25	109.7	-0.3	+1.5 ; -5.0
Slow	200	129.5	-0.1	±1.0
	2	109.9	-0.1	+1.0 ; -5.0
LAE	200	130.0	0.0	±1.0
	2	110.0	0.0	+1.0 ; -2.5
	0.25	100.9	-0.1	+1.5 ; -5.0

Function : 9. Peak C sound level

Number of cycles in test signal	Anticipated Value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
Complete cycle	135.4	134.8	-0.6	±3.0
Positive half cycle	134.4	134.1	-0.3	±2.0
Negative half cycle	134.4	134.1	-0.3	±2.0

Function : 10. Overload indication

Measured value (dB)		Deviated value (dB)	Acceptance limits (dB)
Positive one-half cycle	Negative one-half cycle		
145.3	145.2	-0.1	±1.5

เอกสารไม่ควบคุม

Page 5 of 6

F-CAL-005 Ed.1



ELECTRICAL AND ELECTRONICS INSTITUTE
FOUNDATION FOR INDUSTRIAL DEVELOPMENT

Certificate No.: CP20240292EA

Calibration Report

Function : 11. High-Level Stability

High-level stability over 5 minutes, with steady 1 kHz signal, 1 dB below upper boundary.

Time Period to Apply Signal (min)	Reference SPL (dB)	Record SPL at Conclusion of Time Period (dB)	Deviated value (dB)	Acceptance limits (dB)
5	139.0	139.0	0.0	±0.3

Uncertainty of measurement

Function	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1) Indication at the calibration check frequency	0.30	Not applicable
2) Self-generated Noise	0.10	Not applicable
3) Acoustical signal tests of frequency weightings - Free-field sound pressure response level	0.30	0.60 (10Hz to 4kHz) 0.70 (>4kHz to 10kHz)
4) Electrical signal tests of frequency weightings	0.20	0.20
5) Frequency and time weighting at 1 kHz	0.20	0.20
6) Long-Term Stability	0.10	0.10
7) Level Linearity on the reference level range	0.30	0.30
8) Tone burst response	0.20	0.30
9) Peak C sound level	0.20	0.55
10) Overload indication	0.20	0.25
11) High-Level Stability	0.10	0.10

- Remarks:
- Indication at the calibration check frequency can not measured because customer does not provide a sound calibrator.
 - The acceptance limit is for the deviated value.
 - Acceptance limits was IEC61672-3:2013 Class 2.
 - The coverage factor $k = 2.00$

-- End of Report --

Page 6 of 6

F-CAL-005 Ed.1

เอกสารไม่ควบคุม

INNOVATIVE INSTRUMENT CALIBRATION LAB

INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE

7/19 MOO 13, SOI SUTSAKORN 11 TAMBON BANG KAEU,

AMPHOE BANG PHU SAMUT PRAKARN PROVINCE 10540 THAILAND

TEL : 0669-2116-5900-1 FAX: 0669-2116-7140



Page 1/17

Certificate of Calibration

Customer

Name : UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.
Address : 81 Soi Udonnuk 41, Sukhumvit Road, Bangchak, Prakanong, Bangkok 10260

Certificate No : 24-SLM-237

Request No : Req-2024-1456

Unit Under Calibration Details

Measurement item : Sound Level Meter
Manufacturer : Larson Davis
Model : LX72
Serial Number : 0005193
ID : UAE-EFM-030-2564
Resolution : 0.1 dB
Microphone Class : 2
Microphone Model : 375A04
Microphone S/N : 329354
Preamplifier Model : PRMLX72C
Preamplifier S/N : 073808
Instrument Status : Used

Calibration Environment and Details

Temperature : 23 °C ± 1 °C
Humidity : 50 %RH ± 20 %RH
Barometric Pressure : 1013 hPa ± 10 hPa
Received Date : 1 July 2024
Calibrated Date : 10 July 2024
Calibration Procedure : In-house method CP-SLM-01 based on IEC 61672-3:2013 Electroacoustics - Sound level meters - Part 3: Periodic tests
Location of Calibration : Lab Acoustic

Reference Standard

Instrument	Brand	Model	SN	Due calibration	Traceability
Standard Microphone	GRAS	40AN	188273	20 August 2024	GRAS
Multifrequency Calibrator	Quest	Quest-cal	EFA000234	26 July 2024	TSI
Audio Generator	Svanteck	Svan401	131	8 October 2024	WK Electric

Note

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor $k = 2$, providing a level of confidence approximately 95 %.

Calibrated By :

Mr. Noppadon Luangrat
Service Calibration Engineer

Approved By :

Mr. Pacht Marhavorn
Calibration Engineer Supervisor

Issue Date : 10 July 2024

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Calibration Laboratory.

เอกสารไม่ควบคุม

ISM-700-SLM-01 Rev.04 Issue date 5/6/24

INNOVATIVE INSTRUMENT CALIBRATION LAB

INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE

7/19 MOO 13, SOI SUTSAKORN 11 TAMBON BANG KAEU,

AMPHOE BANG PHU SAMUT PRAKARN PROVINCE 10540 THAILAND

TEL : 0669-2116-5900-1 FAX: 0669-2116-7140



Page 2/7

Certificate No : 24-SLM-237

Request No : Req-2024-1456

1. Indication at the calibration check frequency

UUC Setting Level	Nominal Level (dB)	Before Adjust			After Adjust			UNCERTAINTY (± dB)	Acceptance Limit (± dB)	Result
		UUC (dB)	ERR (dB)	ERR (dB)	UUC (dB)	ERR (dB)	ERR (dB)			
Calibrator Setting										
1000 Hz 114 dB	113.76	114.3	0.54		113.8	+0.04		0.20	0.30	Pass

Note : Absolute sensitivity was established by the use of Sound Calibrator Brand SVANTEK, Model SV 35A, SN: 58079

2. Self-generated noise, Microphone installed

UUC Setting Level	Measured (dB)	UNCERTAINTY (± dB)
FAST / 37-139		
UUC Weighting		
A	28.7	0.10

3. Self-generated noise, Microphone replaced by the electrical input signal device

UUC Setting Level	Measured (dB)	UNCERTAINTY (± dB)
FAST / 37-139		
UUC Weighting		
A	28.4	0.10
C	28.4	0.10
Z	32.9	0.10

4. Acoustic signal test of frequency weightings (Without Windscreen)

UUC Setting	Deviation from various Frequency Weighting Response curve			UNCERTAINTY (± dB)	Acceptance Limit (± dB)	Result
	A	C	Z			
FAST / 37-139						
STD Setting						
125 Hz	0.0	0.1	0.1	0.60	1.5	Pass
1000 Hz	0.0	0.0	0.0	0.60	1.0	Pass
4000 Hz	0.6	0.6	0.6	0.80	3.0	Pass
8000 Hz	0.3	0.3	0.4	0.70	5.0	Pass

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Calibration Laboratory.

เอกสารไม่ควบคุม

ISM-700-SLM-01 Rev.04 Issue date 5/6/24

INNOVATIVE INSTRUMENT CALIBRATION LAB

INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE

7/19 MOO 13, SOI SUTSAKORN 11 TAMBON BANG KAEU,

AMPHOE BANG PHU SAMUT PRAKARN PROVINCE 10540 THAILAND

TEL : 0669-2116-5900-1 FAX: 0669-2116-7140



Page 3/7

Certificate No : 24-SLM-237

Request No : Req-2024-1456

5. Electrical signal test of frequency weightings, Weighting network response with relative to 1 kHz

UUC Setting	Deviation from various Frequency Weighting Response curve			UNCERTAINTY (± dB)	Acceptance Limit (± dB)	Result
	A (dB)	C (dB)	Z (dB)			
FAST / 37-139						
STD Setting						
63 Hz	-0.1	0.0	0.0	0.20	2.0	Pass
125 Hz	-0.1	0.0	0.0		1.5	Pass
250 Hz	-0.1	0.0	0.0		1.5	Pass
500 Hz	0.0	0.0	0.0		1.5	Pass
1000 Hz	0.0	0.0	0.0		1.0	Pass
2000 Hz	0.0	0.1	0.0		2.0	Pass
4000 Hz	0.0	0.0	0.0		3.0	Pass
8000 Hz	0.0	0.0	0.0		5.0	Pass
16000 Hz	-0.1	-0.1	-0.1		+5, -INF	Pass

6. Frequency and time weightings at 1kHz

UUC Setting	STD REF	Measured		UNCERTAINTY (± dB)	Acceptance Limit (± dB)	Result
		UUC (dB)	ERR (dB)			
FAST / 37-139						
UUC Weighting						
A	114.00	114.0	0.0	0.20	0.20	Pass
C	114.00	114.0	0.0		0.20	Pass
Z	114.00	114.0	0.0		0.20	Pass
UUC Time Response						
Fast	114.00	114.0	0.0	0.20	0.10	Pass
Slow	114.00	114.0	0.0		0.10	Pass
Log	114.00	114.0	0.0		0.10	Pass

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Calibration Laboratory.

เอกสารไม่ควบคุม

ISM-700-SLM-01 Rev.04 Issue date 5/6/24

Certificate No : 24-SLM-237
Request No : Req-2024-1456

7. Long Term Stability

UUC Setting	Measured	UNCERTAINTY	Acceptance	Result
FAST / A / 37-139	UUC	(± dB)	Limit (± dB)	
STD Setting	(dB)			
Initial	114.0			
Final	114.0			
Deviated	0.0	0.10	0.30	Pass

8. Level linearity on the reference level range

UUC Setting	Anticipated	Deviation		UNCERTAINTY (± dB)	Acceptance	Result
FAST / A / 37-139	REF	UUC	ERR		Limit	
STD dB	(dB)	(dB)	(dB)		(± dB)	
139.00	139	139.0	0.0	0.30	1.1	Pass
134.00	134	134.0	0.0		1.1	Pass
129.00	129	129.0	0.0		1.1	Pass
124.00	124	124.0	0.0		1.1	Pass
119.00	119	119.0	0.0		1.1	Pass
114.00	114	114.0	0.0		1.1	Pass
109.00	109	109.0	0.0		1.1	Pass
104.00	104	104.0	0.0		1.1	Pass
99.00	99	99.0	0.0		1.1	Pass
94.00	94	94.0	0.0		1.1	Pass
89.00	89	89.0	0.0		1.1	Pass
84.00	84	84.0	0.0		1.1	Pass
79.00	79	79.0	0.0		1.1	Pass
74.00	74	74.0	0.0		1.1	Pass
69.00	69	69.0	0.0		1.1	Pass
64.00	64	64.0	0.0		1.1	Pass
59.00	59	59.0	0.0		1.1	Pass
54.00	54	54.0	0.0		1.1	Pass
49.00	49	49.0	0.0		1.1	Pass
44.00	44	44.1	0.1		1.1	Pass
39.00	39	39.4	0.4		1.1	Pass
34.00	38	38.5	0.5		1.1	Pass

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of **เอกสารไม่ควบคุม**
ISM-709-SLM-01 Rev.04 Issue date 5/6/24

Certificate No : 24-SLM-237
Request No : Req-2024-1456

9. Level linearity including the level range control

UUC Setting	STD	Measured		UNCERTAINTY	Acceptance	Result
FAST / A		REF	UUC		ERR	
UUC Range	(dB)	(dB)	(dB)	(± dB)	(± dB)	
37-139	43.80	43.9	0.1	0.30	1.1	Pass
	114	114.0	0.0		1.1	Pass

10. Tone burst response

UUC Setting	STD	Anticipated	Measured		UNCERTAINTY (± dB)	Acceptance	Result
A / 37-139	Toneburst	Ref	UUC	ERR		Limit (± dB)	
UUC Time Response	(ms)	(dB)	(dB)	(dB)			
Fast	200	135.0	134.9	-0.1	0.20	1.0	Pass
	2	118.0	117.9	-0.1		+1.0, -2.5	Pass
	0.25	109.0	108.7	-0.3		+1.5, -3.0	Pass
Slow	200	128.6	128.4	-0.2		1.0	Pass
	2	109.0	108.8	-0.2		+1.0, -5.0	Pass
	200	129.0	129.0	0.0		1.0	Pass
SEL	2	109.0	109.1	+0.1	+1.0, -2.5	Pass	
	0.25	100.0	99.9	-0.1	+1.5, -5.0	Pass	

11. Peak C Sound level

UUC Setting	Anticipated	Measured		UNCERTAINTY	Acceptance	Result
FAST / C / 95-142	REF	UUC	ERR	(± dB)	Limit	Result
STD Setting	(dB)	(dB)	(dB)		(± dB)	
Complete cycle	137.4	136.8	-0.60		3.0	Pass
Positive half cycle	136.4	136.2	-0.20	0.20	2.0	Pass
Negative half cycle	136.4	136.2	-0.20		2.0	Pass

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of **เอกสารไม่ควบคุม**
ISM-709-SLM-01 Rev.04 Issue date 5/6/24

Certificate No : 24-SLM-237
Request No : Req-2024-1456

12. Overload indication

UUC Setting	Measured	UNCERTAINTY	Acceptance	Result
FAST / A / 37-139	UUC	(± dB)	Limit (± dB)	
STD Setting	(dB)			
Positive one-half cycle	142.6			
Negative one-half cycle	142.6			
Deviated	0.0	0.20	1.5	Pass

13. High Level Stability

UUC Setting	Measured	UNCERTAINTY	Acceptance	Result
FAST / A / 37-139	UUC	(± dB)	Limit (± dB)	
STD Setting	(dB)			
Initial	138.0			
Final	138.0			
Deviated	0.0	0.10	0.30	Pass

Note :

Function	Maximum-permitted Uncertainty of measurement
1. Indication at the calibration check frequency	Not applicable
2. Self-generated noise, Microphone installed	Not applicable
3. Self-generated noise, Microphone replaced by the electrical input signal device	Not applicable
4. Acoustic signal test of frequency weightings at 10 Hz to 4 kHz	0.80 dB
4. Acoustic signal test of frequency weightings at >4 kHz to 10 kHz	0.70 dB
5. Electrical signal test of frequency weightings, Weighting network response with relative to 1 kHz	0.20 dB
6. Frequency and time weightings at 1 kHz	0.26 dB
7. Long Term Stability	0.10 dB
8. Level linearity on the reference level range	0.30 dB
9. Level linearity including the level range control	0.30 dB
10. Tone burst response	0.30 dB
11. Peak C Sound level	0.35 dB
12. Overload indication	0.25 dB
13. High Level Stability	0.10 dB

- Acceptance Limit and Maximum-permitted Uncertainty was IEC 61672-1:2013.

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of **เอกสารไม่ควบคุม**
ISM-709-SLM-01 Rev.04 Issue date 5/6/24

Certificate No : 24-SLM-237
Request No : Req-2024-1456

Decision Rule for Statements of Conformity


The standard decision rule employ for the statements of conformity to each calibration result will be applied using ILAC-G8/09:2019, Guidelines on the Reporting of Compliance with Specification as following Fig. and statements

Pass - The measurement result plus the expanded uncertainty with a 95% coverage probability were within the limit.

Pass¹ - The measurement result was within the limit. However, a portion of the expanded uncertainty of measurement at 95% exceeds the limit.

Fail¹ - The measurement result was out of the limit. However, a portion of the expanded uncertainty of measurement at 95% is within the limit.

Fail - The measurement result plus the expanded uncertainty with a 95% coverage probability were outside the limit.

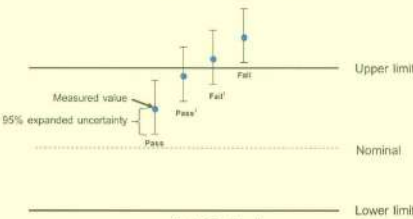

End of Certificate

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of **เอกสารไม่ควบคุม**
ISM-709-SLM-01 Rev.04 Issue date 5/6/24



Certificate No.: CP20240291EA
Operation No.: CP2024070254

Certificate of Calibration

Equipment: Sound Level Meter

Manufacturer: Larson Davis (Meter), PCB (Microphone), PCB (Preamplifier)

Model/Type: LxT2 (Meter), 375A04B02 (Microphone), PRLxT2C (Preamplifier)

Serial No.: 0005396 (Meter), 329350 (Microphone), 073805 (Preamplifier)

ID No.: UAE.EFM.033/2564

Customer: United Analyst and Engineering Consultant Co.,Ltd.

Address: 81 Soi Udomsuk 41, Sukhumvit Road, Bangchak
Phrakhanong, Bangkok 10260

Received Date: 25 July 2024

Calibrated Date: 5 - 6 August 2024

Issued Date: 7 August 2024

Calibrated by: Ms. Juntaporn Kunhakom

Approved by: 
(Mr. Sittichai Swaksuriyawong)
Group Manager

This report was prepared electronically using applicable electronic signature. Printing or copy of file are considered as a copy of the document.
The reported uncertainty of measurement was based on standard uncertainty multiplied by a coverage factor (k)
providing a level of confidence of approximately 95%. This certificate may not be reproduced other than in full except
with the prior written approval of the Electrical and Electronics Institute, Foundation for Industrial Development.

Page 1 of 6

เอกสารไม่ควบคุม

F-CAL-004 Ed.1



Certificate No.: CP20240291EA

Calibration Report

Equipment: Sound Level Meter

Manufacturer: Larson Davis (Meter), PCB (Microphone), PCB (Preamplifier)

Model/Type: LxT2 (Meter), 375A04B02 (Microphone), PRLxT2C (Preamplifier)

Serial No.: 0005396 (Meter), 329350 (Microphone), 073805 (Preamplifier)

ID No.: UAE.EFM.033/2564

Ambient Temperature: (23 ± 2) °C

Relative Humidity: (50 ± 15) %

Pressure: (101.3 ± 1.5) kPa

Method of Calibration :-
IEC 61672-3:2013.

Condition of this result of calibration

1. Reference standards instrument :-

	Instrument	Model	Serial No.	Cert. No.	Due Date
1)	Standard microphone	4180	2787490	AA-1012-23	12 November 2024
2)	Arbitrary Function Generator	AFG2021	C010063	CK20240048EA	23 June 2025
3)	Programmable Attenuator	PA5	2755	EF-0040-23	1 October 2024
4)	6.5 Digit precision multimeter	8846A	9610014	CB20230200EA	15 November 2024
5)	Pressure humidity and Temperature Transmitter	PTU301	L3950483	CL1-P240023 CD20240142EA	24 March 2025 12 June 2025
6)	Pressure humidity and Temperature Transmitter	PTU301	L3950484	CL1-P240030 CD20240143EA	11 April 2025 12 June 2025
7)	Performance Audio Analyzer	U89038	MY56510003	CB20240035EB CK20230072EA	13 February 2025 13 September 2024

2. This result of calibration was found accurate as shown on date and place of calibration only.

3. This certification is traceable to the international system of unit maintained at :-

Reference standards instrument for Acoustic function

- National Institute of Metrology (Thailand)

Reference standards instrument for Electrical function

- National Institute of Metrology (Thailand)

- Electrical and Electronics Institute; NSC Accredited Calibration No.0119

Result of Calibration:-

Function : 1. Indication at the calibration check frequency

Reference Acoustic Signal (dB)	Measured value (dB)	Deviation (dB)	Acceptance limits (dB)
-	-	-	-

Page 2 of 6

F-CAL-005 Ed.1

เอกสารไม่ควบคุม



Certificate No.: CP20240291EA

Calibration Report

Function : 2. Self-generated Noise
2.1 Microphone Installed

Measured value (dB)
29.3

2.2 Microphone replaced by the electrical input signal device

Frequency Weighting	Measured value (dB)
A-weighting	29.1
C-weighting	28.8
Z-weighting	34.1

Function : 3. Acoustical signal tests of frequency weightings (Without Windscreen)

Meter free-field acoustic response at a level of 84 dB.

Frequency (Hz)	Deviation from various Frequency Weighting Response Curve			
	C-Weighting (dB)	A-Weighting (dB)	Z-Weighting (dB)	Acceptance limits (dB)
125	0.3	0.1	0.3	±1.5
1000	-0.1	-0.1	-0.1	±1.0
8000	0.2	0.2	0.2	±5.0

Function : 4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various Frequency Weighting Response Curve			
	C-Weighting (dB)	A-Weighting (dB)	Z-Weighting (dB)	Acceptance limits (dB)
63	0.0	0.0	0.0	±2.0
125	0.0	0.0	0.0	±1.5
250	0.0	0.0	0.0	±1.5
500	0.0	0.0	0.0	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.0	0.0	±2.0
4000	0.0	0.0	0.0	±3.0
8000	0.0	-0.1	0.0	±5.0

Function : 5. Frequency and time weighting at 1 kHz

5.1 Frequency weighting at 1 kHz

Frequency Weighting	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
C-weighting	94.0	0.0	±0.2
A-weighting	94.0	0.0	±0.2
Z-weighting	94.0	0.0	±0.2

เอกสารไม่ควบคุม

Page 3 of 6

F-CAL-005 Ed.1



Certificate No.: CP20240291EA

Calibration Report

5.2 Time weighting at 1 kHz

Time Weighting	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
Fast	94.0	0.0	±0.1
Slow	94.0	0.0	±0.1
LAeq	94.0	0.0	±0.1

Function : 6. Long-Term Stability

Long-term stability over 30 minutes, with steady 1 kHz signal at reference level.

Time Period to Apply Signal (min)	Reference SPL (dB)	Record SPL at Conclusion of Time Period (dB)	Deviated value (dB)	Acceptance limits (dB)
30	94.0	94.0	0.0	±0.3

Function : 7. Level Linearity on the reference level range

7.1 Level Linearity on the reference level range, Upper

Anticipated Value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
94.0	94.0	0.0	±1.1
99.0	99.0	0.0	±1.1
104.0	104.0	0.0	±1.1
109.0	109.0	0.0	±1.1
114.0	114.0	0.0	±1.1
119.0	119.0	0.0	±1.1
124.0	124.0	0.0	±1.1
129.0	129.0	0.0	±1.1
134.0	134.1	0.1	±1.1
139.0	139.1	0.1	±1.1
140.0	140.1	0.1	±1.1
141.0	141.1	0.1	±1.1

เอกสารไม่ควบคุม

Page 4 of 6

F-CAL-005 Ed.1

Certificate No.: CP20240291EA

Calibration Report

7.2 Level Linearity on the reference level range, Lower

Anticipated Value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
94.0	94.0	0.0	±1.1
89.0	89.0	0.0	±1.1
84.0	84.0	0.0	±1.1
79.0	79.0	0.0	±1.1
74.0	74.0	0.0	±1.1
69.0	69.0	0.0	±1.1
64.0	64.0	0.0	±1.1
59.0	59.0	0.0	±1.1
54.0	54.0	0.0	±1.1
49.0	49.0	0.0	±1.1
44.0	44.1	0.1	±1.1
43.0	43.1	0.1	±1.1
42.0	42.2	0.2	±1.1
41.0	41.2	0.2	±1.1
40.0	40.3	0.3	±1.1

Function : 8. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
Fast	200	135.9	-0.1	±1.0
	2	118.8	-0.2	+1.0 ; -2.5
	0.25	109.8	-0.2	+1.5 ; -5.0
Slow	200	129.5	-0.1	±1.0
	2	109.9	-0.1	+1.0 ; -5.0
	0.25	101.0	0.0	+1.5 ; -5.0

Function : 9. Peak C sound level

Number of cycles in test signal	Anticipated Value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
Complete cycle	135.4	134.8	-0.6	±3.0
Positive half cycle	134.4	134.0	-0.4	±2.0
Negative half cycle	134.4	134.0	-0.4	±2.0

Function : 10. Overload indication

Measured value (dB)		Deviated value (dB)	Acceptance limits (dB)
Positive one-half cycle	Negative one-half cycle		
143.4	143.4	0.0	±1.5

Page 5 of 6

F-CAL-005 Ed.1

เอกสารไม่ควบคุม

Certificate No.: CP20240291EA

Calibration Report

Function : 11. High-Level Stability

High-Level stability over 5 minutes, with steady 1 kHz signal, 1 dB below upper boundary.

Time Period to Apply Signal (min)	Reference SPL (dB)	Record SPL at Conclusion of Time Period (dB)	Deviated value (dB)	Acceptance limits (dB)
5	139.0	139.0	0.0	±0.3

Uncertainty of measurement

Function	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1) Indication at the calibration check frequency	0.30	Not applicable
2) Self-generated Noise	0.10	Not applicable
3) Acoustical signal tests of frequency weightings - Free-field sound pressure response level	0.30	0.60 (10Hz to 4kHz) 0.70 (>4kHz to 10kHz)
4) Electrical signal tests of frequency weightings	0.20	0.20
5) Frequency and time weighting at 1 kHz	0.20	0.20
6) Long-Term Stability	0.10	0.10
7) Level Linearity on the reference level range	0.30	0.30
8) Tone burst response	0.20	0.30
9) Peak C sound level	0.20	0.35
10) Overload indication	0.20	0.25
11) High-Level Stability	0.10	0.10

- Remarks:
1. Indication at the calibration check frequency can not measured because customer does not provide a sound calibrator.
 2. The acceptance limit is for the deviated value.
 3. Acceptance limits was IEC61672-3:2013 Class 2.
 4. The coverage factor $k = 2.00$

-- End of Report --

Page 6 of 6

F-CAL-005 Ed.1

เอกสารไม่ควบคุม



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000-29 FAX. 0-2719-9484



Cert.No.: 24CH239
Page.: 1 of 3

Certificate of Calibration

Equipment : pH Meter
Manufacturer : Horiba
Model : LAQUA-PH210
Serial No. : HA0D0078
ID No. : UAE.EFM.073/2564(EFM.pH.06/64)
Condition As-Received: Used Item
Received Date : 19 February 2024
Calibration Date : 20 February 2024
Reference : 2402-0594WSC-3
Submitted by : United Analyst and Engineering Consultant Co.,Ltd.
3 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Ambient Temperature : (25 ± 2.5) °C
Relative Humidity : (50 ± 15) %
Calibration Procedure : In-house method :
- CP-CH5 by direct measurement with DC Voltage Standard and direct measurement with certified reference material (CRM)
- CP-CH8 by comparison with temperature standard

Calibrated by : Walalak Sirthean

Approved by : 
Approved Signatory

() Pornthippa Tameyakul
() Unnophol Harachai
(✓) Salthip Meangmai

Issue Date : 22 February 2024

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3: Equipment Calibration and Testing Services.

เอกสารไม่ควบคุม

A 0063841



Cert.No.: 24CH239
Page.: 2 of 3

Condition of this calibration result

1. Reference Standard Instrument

Instrument	Serial No.	ID No.	Cert. No.	Due Date
1) Document Process Calibrator	54030049	130RC116	23E2802	27 Aug 2024
2) Ref. Standard Thermometer	4982054	110RC044	23I908	26 July 2024

This certification is traceable to the International System of Unit maintained through:-
- Technology Promotion Association (Thailand-Japan)

2. Certified Reference Materials : The measurement results are traceable to SI through CPA chem Ltd.,
ANSI-ASQ National Accreditation Board, Accredited No. AR-1835

Buffer Solution	Manufacturer	Lot No.	Exp. date
pH 4.008	CPA chem	940102	27 Nov 2025
pH 6.986	CPA chem	940104	02 Nov 2024
pH 9.997	CPA chem	940106	02 Nov 2024

3. This certificate is valid only to the item calibrated on date and place of calibration.

Calibration Results

Function : mV Measurement

Performing standard curve by Document Process Calibrator at pH (4.7)(7,10)

Unit Under Calibration	Nominal Value	Standard Voltage Input		Actual Reading		Uncertainty of Measurement (±mV)	Coverage factor k
	pH	mV		mV	pH		
pH Meter S/N.: HA0D0078	4.00	177.48		177.4	4.01	0.058	2.00
	7.00	0.00		0.0	7.00	0.058	2.00
	7.00	0.00		0.0	7.00	0.058	2.00
	10.00	-177.48		-177.5	10.01	0.058	2.00

เอกสารไม่ควบคุม

a 1203292



Cert.No.: 24CH239
Page.: 3 of 3

Calibration Results

Function : pH Measurement

Performing three buffers standard curve by using buffer nominal pH (4,7)(7,10)

Unit Under Calibration	Standard pH Buffer Solution	Actual pH Reading	Actual mV Reading (mV)	Uncertainty of pH Measurement (\pm)	Coverage factor k
pH Electrode S/N.: 992H0385	4.008	4.02	168.3	0.0086	2.05
	6.986	6.99	-7.7	0.0093	2.00
	6.986	6.99	-7.6	0.011	2.00
	9.997	10.01	-180.7	0.0085	2.00

Function : Temperature Measurement

(*) Without adjustment

This equipment was connected with Temperature Probe;

- Model : 9652
- Serial No. : 992H0385

Dimension of probe

- Length : 110 mm.
- Diameter : 16 mm.
- Immersion Depth : 100 mm.

Calibration Point (°C)	Standard Temperature (°C)	UUC* Reading (°C)	Error (°C)	Uncertainty of measurement (\pm °C)	Coverage factor k
25.0	25.000	25.0	0.000	0.13	2.00
30.0	30.000	30.0	0.000	0.13	2.00
35.0	34.999	35.0	0.001	0.13	2.00

Remark - UUC* = Unit Under Calibrator

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k , providing a level of confidence of approximately 95 %.

-o0o-

เอกสารไม่ควบคุม

a 1203291