

ภาคผนวก ง

สำเนาเอกสารการสอบเทียบเครื่องมือตรวจวัด

ภาคผนวก ง-1

ใบรับรองสอบเทียบเครื่องมือตรวจวัดคุณภาพอากาศ
ในบรรยากาศ



National Institute of Metrology (Thailand)

Ministry of Higher Education, Science, Research and Innovation

Certificate of Calibration

Certificate No. : MW-0036-24
Issued by : Flow and Volume of Liquid Laboratory
Mechanical Metrology Department

Page 1 of 3 pages

MEASUREMENT ITEM : Orifice Gas Flow Device

MANUFACTURER : Tisch Environmental, Inc.

MODEL/TYPE : TE-5025A

SERIAL NUMBER : 0992

CUSTOMER : ENVIPRO CO.,LTD.
168/28,168/30,168/71 Nakniwat Rd., Lat Phrao District,
Lat Phrao District, Bangkok 10230

MEASUREMENT DATE : April 4, 2024

The reported measurement result relates only to the measurand and applies only at the time of measurement.

Reference:
MEC9734-01/24

Date:
April 5, 2024

Approved by:

(Wirun Laopornpichayanuwat)

Performed by:

(Terdsak Neadkratoke)

Partial reproduction of this certificate is permitted only with a written permission from NIMT.



ENVIRONMENTAL CONDITIONS:

Ambient condition in the laboratory are as follows :

Temperature	: 23.0 ± 2.0	°C
Relative Humidity	: 55 ± 15	%RH

Calibration Condition:

Preconditioning	: 24 hours at ambient conditions.
Measurement Condition	: The average values during measurement are 23.3°C and 57 %RH.

MEASUREMENT METHOD:

The Orifice gas flow device was calibrated against NIMT's Standard Gas Meter Model DELTA S-Flow G65. The CP-MW 0009 was used as a calibration guideline.

TABULATION OF RESULTS:

The tables on the next page give the measured values.

UNCERTAINTY OF MEASUREMENT:

The stated uncertainty is the expanded uncertainty which is obtained by multiplying the standard uncertainty by the coverage factor $k = 2$. It has been determined in accordance with EA publication EA-4/02M:2013 "Evaluation of the Uncertainty of Measurement in Calibration" and "JCGM 100:2008 Evaluation of measurement data - Guide to the Expression of Uncertainty in Measurement (GUM 1995 with minor corrections)". The value of the measurand lies within the assigned range of values with a probability of 95 %.

TRACEABILITY:

This certificate provides a traceability of the measurement to recognized the national standards, and to the realization of the International System of Units (SI).



MEASUREMENT RESULTS:

The Orifice gas flow device was calibrated by direct comparison method with the Gas Meter standard. The Humid air was used as a medium in the system. The standard conditions are 25°C (298.15 K) and 760 mmHg for standard temperature and standard pressure respectively.

Table 1. The results of Q actual calibration data

Plate	Flow rate m^3/min	Pressure [Pa] mmHg	Temperature [Ta] °C	Temperature [Tm] °C	Δp _Meter mmHg	Δp _Orifice inH ₂ O	Y	Actual Flow [Q_a] m^3/min
1	0.696	756.770	23.61	23.64	5.663	1.866	0.855	0.691
2	0.910	756.782	23.67	23.69	9.001	3.147	1.111	0.899
3	0.993	756.792	23.74	23.70	10.500	3.731	1.210	0.979
4	1.067	756.812	23.76	23.61	11.930	4.292	1.298	1.051
5	1.164	756.799	23.74	23.46	13.921	5.077	1.411	1.143

Slope (m): 1.22951

Intercept (b): 0.00554

Correlation coefficient (r): 0.99994

Uncertainty ($k=2$): 0.015 m^3/min

Table 2. The results of Q standard calibration data

Plate	Flow rate m^3/min	Pressure [Pa] mmHg	Temperature [Ta] °C	Temperature [Tm] °C	Δp _Meter mmHg	Δp _Orifice inH ₂ O	Y	Standard Flow [Q_{std}] m^3/min
1	0.696	756.770	23.61	23.64	5.663	1.866	1.366	0.691
2	0.910	756.782	23.67	23.69	9.001	3.147	1.774	0.899
3	0.993	756.792	23.74	23.70	10.500	3.731	1.931	0.979
4	1.067	756.812	23.76	23.61	11.930	4.292	2.072	1.051
5	1.164	756.799	23.74	23.46	13.921	5.077	2.253	1.143

Slope (m): 1.96301

Intercept (b): 0.00885

Correlation coefficient (r): 0.99994

Uncertainty ($k=2$): 0.016 m^3/min

End of Certificate of Calibration

CERTIFICATE OF CALIBRATION

Certificate No.: B1-2602012/24

Page 1 **of total** 5 **pages**

Customer ENVIRPRO CO., LTD.

168/28 Nakniwas Rd., Ladprao, Bangkok 10230

Equipment Electronic Balance

Manufacturer AND

Model HR-202i

Serial No. 15201052

ID No. SV-TL.044/2559

Description Maximum Capacity: 50 g

Resolution: 0.00001 g

Maximum Capacity: 220 g

Resolution: 0.0001 g

Environmental Conditions Ambient Temperature: 27.4 °C

Relative Humidity: 44.5 %

Atmospheric Pressure: -

Calibration Location ห้องเครื่องชั่ง

Received Date 26 February 2024

Calibration Date 26 February 2024

Date of Issue 27 February 2024

Condition of Artifacts Used conditions but can be calibrated

Checked by



Act as Technical Manager

Approved by



Representative of Managing Director

- | | |
|---|--|
| <input type="checkbox"/> (Krisyosl K.) | <input type="checkbox"/> (Sakda Y.) |
| <input type="checkbox"/> (Patiphan K.) | <input type="checkbox"/> (Onnapa P.) |
| <input type="checkbox"/> (Pongsak H.) | <input type="checkbox"/> (Nitiphong K.) |
| <input checked="" type="checkbox"/> (Kanung C.) | <input type="checkbox"/> (Nonthachai K.) |
| <input type="checkbox"/> (Pramong P.) | <input type="checkbox"/> (Noppol P.) |

(Dr. Ekachai Puttitwong)

This calibration certificate shall not be reproduced other than in full except with the prior written approval of the Thai Heart Calibration Co., Ltd.

Certificate No.: B1-2602012/24

Page 2 of total 5 pages

Reference Method:

- The calibration method used was CP-208 based on UKAS LAB 14
- This certificate can be traceable to the national standards, which is realized the shown measurement units according to the International System of Units (SI Units).

Reference Standard Instruments:

Type	Model	Serial No.	Cert. No.	Due Date	Traceability
Standard Weight Set 1 mg - 200 g	-	158841	MM-0032-22	Mar. 15, 2024	NIMT

Remark: This certificate is traceable to the International System of Unit (SI Unit) through:

- NIMT, National Institute of Metrology (Thailand).

Measurement Results:

- ☒ Without Adjustment
☐ After Adjustment

1. Repeatability


Nominal Weight	Standard Deviation of Reading (g)
200 g	0.00003

Certificate No.: B1-2602012/24


Page 3 of total 5 pages

Measurement Results (Cont.):

2. Off-Center Loading



Front

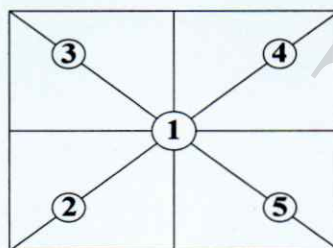

Front



Measuring Positions

Measuring Positions	Instrument Reading (g)	Max. Difference (g)
1	50.00006	0.00046
2	50.00023	
3	49.99998	
4	49.99977	
5	50.00018	
1	50.00005	

3. Error of indication from nominal value

Standard Weight (g)	Instrument Reading (g)		Correction (g)	Uncertainty of Measurement (g)
	Without Adjustment	After Adjustment		
0.00100	0.00099	-	0.00001	± 0.000043
0.00300	0.00303	-	-0.00003	± 0.000044
0.00500	0.00499	-	0.00001	± 0.000043
0.01000	0.00999	-	0.00001	± 0.000044
0.05000	0.05000	-	0.00000	± 0.000044
0.10000	0.09999	-	0.00001	± 0.000044
0.50000	0.50002	-	-0.00002	± 0.000045
1.00000	1.00004	-	-0.00004	± 0.000045
9.99998	10.00001	-	-0.00003	± 0.000052
19.99997	20.00012	-	-0.00015	± 0.000062
29.99995	30.00011	-	-0.00016	± 0.000074
40.00000	40.00014	-	-0.00014	± 0.000074

Calibrated by

Natthapong

Certificate No.: B1-2602012/24

Page 4 of total 5 pages

Measurement Results (Cont.):

3. Error of indication from nominal value (Cont.)

Standard Weight (g)	Instrument Reading (g)		Correction (g)	Uncertainty of Measurement (g)
	Without Adjustment	After Adjustment		
49.99993	50.00007	-	-0.00014	± 0.000081
59.9999	60.0001	-	-0.0002	± 0.00014
69.9999	70.0002	-	-0.0003	± 0.00014
79.9999	80.0001	-	-0.0002	± 0.00014
84.9999	85.0001	-	-0.0002	± 0.00014
89.9999	90.0000	-	-0.0001	± 0.00015
99.9999	99.9998	-	0.0001	± 0.00016
109.9999	109.9999	-	0.0000	± 0.00028
119.9999	119.9999	-	0.0000	± 0.00028
129.9998	129.9999	-	-0.0001	± 0.00028
139.9999	140.0000	-	-0.0001	± 0.00028
149.9998	149.9998	-	0.0000	± 0.00028
159.9998	159.9996	-	0.0002	± 0.00028
169.9998	169.9997	-	0.0001	± 0.00028
179.9998	179.9997	-	0.0001	± 0.00028
189.9998	189.9996	-	0.0002	± 0.00028
199.9999	199.9995	-	0.0004	± 0.00028

Calibrated by Natthapong

Certificate No.: B1-2602012/24

Page 5 of total 5 pages

Measurement Results (Cont.):

4. Effect of Tare

Nominal Tare Weight (g)	Standard Weight (g)		Instrument Reading (g)	Instrument Deviation (g)
50	Tare		0.0000	0.0000
	at 20 %	10.0000	10.0001	0.0001
	at 40 %	20.0000	20.0000	0.0000
	at 60 %	50.0000	49.9998	-0.0002
	at 80 %	100.0000	99.9996	-0.0004
	at 100 %	150.0000	149.9993	-0.0007

The above reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor $k = 2.00$, providing a level of confidence approximately 95%.

- End of Certificate -

GC Clarus 500/580 Preventive Maintenance (PM)

Company Name:			
Address (Instrument Location):			
Serial Number:		Service Tag:	
Customer Name (if applicable):		PM number:	
Service Engineer Name:		Service Order Number:	
Date PM Performed: (DD-MMM-YYYY)		Next PM Due Date: (DD-MMM-YYYY)	

Part Number	Release	Publication Date	
TH09370050	2.2	Jan 2020	

Scope

The purpose of this PM is to ensure the continued functionality of the Clarus 500 and Clarus 580 GC by inspecting and replacing any worn or damaged parts. This service should only be performed by a trained representative of PerkinElmer. The customer should save their method before the PM begins.

General Instructions:

The customer must provide the engineer operational data to demonstrate recent instrument performance prior to starting the PM. Always check with the customer before making any changes that may affect the customer's analysis or calibration, including a current back-up of system software and/or data files. The completed document should be signed by an authorized PerkinElmer and customer representative and left with the customer. Update the PM sticker and instrument logbook as required.

Copyright Information

This document contains proprietary information that is protected by copyright. All rights are reserved. No part of this publication may be reproduced in any form whatsoever or translated into any language without the prior, written permission of Perkin Elmer, Inc. **Copyright © 2013 PerkinElmer, Inc.**

Trademarks

Registered names, trademarks, etc. used in this document, even when not specifically marked as such, are protected by law. PerkinElmer is a registered trademark of PerkinElmer, Inc. All other trademarks and registered trademarks not owned by PerkinElmer, Inc. or its subsidiaries that are depicted herein are the property of their respective owners. **Except as specifically set forth in its terms and conditions of sale, PerkinElmer makes no Warranty of any kind with regard to this document, including, but not limited to, the implied warranties of merchantability and fitness for a particular purpose.** PerkinElmer shall not be liable for incidental or consequential damages in connection with the furnishing or use of this document.

Component List

Component / Specific Model	Serial #	Software Version	Configuration Notes

Parts Lists

Additional Tools Required for PM				
Part Number (if applicable)	Description	Quantity	Serial #	Calibration Due Date (MM/YY)
Additional Reagents and Standards Required for PM				
Part Number (if applicable)	Description	Quantity	Batch/Lot #	Expiration Date (MM/YY)

Procedure Checklist

Use (✓) to check off those steps in the checklist that have been completed.

1. General:

Review the instrument performance with the customer and document any recent problems.

Check incoming AC line voltage for proper levels and grounding.

L-N _____ Volt
L-G _____ Volt
N-G _____ Volt

**Neutral to ground not more than 0.5 volts peak to peak*

Inspect all gas line filters and traps; Replace if necessary with customer supplied spares.

Carrier gas	Helium	Nitrogen	Hydrogen	
Moisture level	Good	Need to replace	Other	_____
Detector gas	Air Zero	Hydrogen	Nitrogen	Helium
Moisture level	Good	Need to replace	Other	_____

Inspect the customer log book and make any appropriate PM entries.

Leak check all fittings from the gas source to instrument.

Gas leakage Pass Fail Comment _____

Perform general inspection of system for cleanliness.

Inspect for functional and clean electronic cooling and oven vent fans

Electronic cooling fan	Yes	No
Oven cooling fan	Yes	No

2. Electronic :

Check oven temperature. Calibrate if necessary.

Oven temperature set point °C Pass Fail

Check sub-ambient option. (If installed).

Oven temperature set point 5 °C Pass Fail

Perform routine maintenance on detector/injector. Replace parts as necessary with customer supplied spares.

Check flows, including split flows if applicable. Calibrate if necessary.

Carrier flow Pass Fail

Split flow

Check detector gas flows and adjust if necessary.

Detector flow Pass Fail

Autosampler installed Yes No

Check autosampler sensor for wear and replace if necessary.

Vial sensor Pass Fail

Door sensor Pass Fail

Tower sensor Pass Fail

Plunger sensor Pass Fail

Elevator sensor Pass Fail

Remove syringe, manually flush. Replace with customer supplied spare if necessary.

Check firmware version. Upgrade to current levels if necessary.

Firmware version _____

Measure all accessible power supply voltages.

5 Volt Pass Fail

+15 Volt Pass Fail

-15 Volt Pass Fail

24 Volt Pass Fail

Record all detector voltage signal.

Detector Channel A _____ mV.

Detector Channel B _____ mV.

3. Diagnostics Tests:

Run instrument diagnostics.

BRAM Pass Fail

EPROM Pass Fail

Run Autosampler diagnostics.

BRAM Pass Fail

EPROM Pass Fail

4. Review:

Review with the customer PM work performed.

Review with the customer routine maintenance procedures.

Discuss recommended customer-supplied materials to have on hand

Attach PM sticker.

Update Logbook.

Additional Comments

Additional Comments Regarding the PM

Review

<p><i>The preventive maintenance checks and if applicable performance tests for Clarus500/580 GC have been completed.</i></p>	
<p><i>This Clarus500/580 GC</i></p>	<p><i>the preventive maintenance.</i></p>
<p>Review of Preventive Maintenance:</p>	
<p>Authorized PerkinElmer Representative:</p> <p><i>Nisan</i></p>	<p>Date:</p> <p>(DD-MMM-YYYY)</p>
<p>Authorized Customer Representative:</p> <p><i>Wank</i></p>	<p>Date:</p> <p>(DD-MMM-YYYY)</p>

Service Report



Work Order Number	Activity Code	Billing Type	Requested Start Date	Model	Serial Number
WO-02928942	Repair	Contract	25/07/2567 10:11 น.	CLARUS500	650N3022702
Service Representative Name	Contract Number	Expiry Date	Equipment ID	System ID	
Inkum, Wisan	SC-0035622058	13/06/2025	N/A	N/A	
UDI Number					
N/A					
Equipment Location			Bill To Name		
บริษัท เอ็นไวร์โปร จำกัด เขตลาดพร้าว กรุงเทพฯ 51 10230 TH			บริษัท เอ็นไวร์โปร จำกัด เขตลาดพร้าว กรุงเทพมหานคร 51 10230 TH		
Customer Contact	Phone Number	Fax Number	Email	Purchase Order	
K. Sasitron	0-2831-6699	0-2831-6698	N/A	6501023	

Work Description		
PM1/2 replace PM kit. add N6101183 Auto sample vial locator spring. 09902143 Silicone rubber O-ring Check flows, including split flows. Check detector gas flows Check Oven temperature Check autosampler sensor Remove syringe, manually flush. Replace with customer supplied spare if necessary. Measure all accessible power supply voltages.		
Start Date	End Date	Work Description
25/07/2024	25/07/2024	
25/07/2024	25/07/2024	
31/07/2024	31/07/2024	
31/07/2024	31/07/2024	

Tools Used					
Quantity	Calibrated Tool	Description	Serial Number	Last Calibration Date	Next Calibration Date
*** No Calibrated Tools Used ***					

Material Used				
Part Number	Part Description	Note	Lot/Serial Number	Quantity
N6101182	Replacement Vial Locator for Autosampler			1
N6121004	Quartz Liner for Spit Operation; 2 mm ID			1
09921004	O-Ring 9.32 OD x 5.32 ID			1
N6001204	Jet Contact Spring for External Igniter			1
N6100432	PIN ASSY-ASXL FID POL			1
N9306873	Blue GC Inlet Septa 10 Pk			1

Labour Details			
Part Number	Part Description	Start Date	Quantity
SV000013	Preventative maintenance	25/07/2024	4
SV000004	Service F.O.C. Travel	25/07/2024	1
SV000013	Preventative maintenance	31/07/2024	2
SV000004	Service F.O.C. Travel	31/07/2024	1

Work Complete		Customer Signature	Technician Signature
Yes	<input checked="" type="checkbox"/>	No	<input type="checkbox"/>
PM/OQ/IPV Left with Customer		 31/7/2567 K. Sasitron	 31/7/2567 Inkum, Wisan
Yes	<input type="checkbox"/>		

Terms & Conditions
<p>Customer Acknowledgment of receipt of the above repair / replacement.</p> <p>Special Terms and Conditions: This is not an invoice.</p> <p>Taxes will be applied to your invoice if applicable.</p>



THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804, 0-2399-0469

Calibration Certificate

Issued by : Calibration & Test Section : Meteorological Instruments Bureau

Date of Issue 11 January, 2024

Certification No. 019/24

Page : 1 of 2

Object : Wind speed and wind direction

Manufacturer : Sensor : NRG
Basic Datalogger : Symphonie

Type : Sensor : #40C Basic Datalogger : LR20

Serial No. : Sensor : 1795-00124576 Basic Datalogger : 30906578

Customer : ENVIRPRO CO.,LTD.
168/28 Nakniwas Rd., Ladprao,
Bangkok 10230.

Calibration Condition : Temperature 25.1 °C Barometric Pressure 1010.4 hPa

NATIONAL STANDARD WIND TUNNEL :

: Micromanometer Theodor Friedrichs FC014 Serial No. 9310119


: HOOK GAGE NO 1425 Pitot Tube Theodor Friedrichs Type 0800.0000 serial 9023


N.I.S.T. Test Reference Number 731/241460 : Standard Velocity at 20 - 30 m/sec


: Ultrasonic Anemometer Model DA-650-3TV (sensor TR-90AH)

Serial Number 110730029 (sensor 120629586)

JAPAN QUALITY ASSURANCE ORGANIZATION : Standard Velocity at 0 - 20 m/sec

Calibrated by : 
Mr. Watcharapol Subwat
Mechanical Engineer

Signed : 
Mr. Pisood Promsut

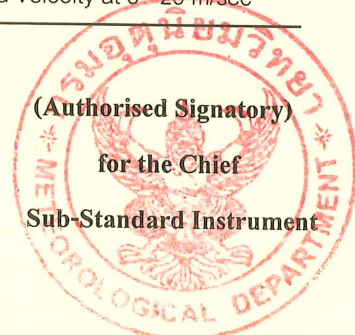



THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804,0-2399-0469

The Result of Calibration

Certification No. 019/24

11 January, 2024

Page : 2 of 2

Standard Ultrasonic Anemometer m/sec	HOOK GAGE NO. 1425			TESTED ANEMOMETER	
	Pressure inches H2O	Vacumm inches H2O	Velocity m/sec	Velocity m/sec	Correction m/sec
1.00	-	-	-	0.85	0.15
3.02	-	-	-	2.98	0.04
5.00	-	-	-	5.07	-0.07
7.04	-	-	-	7.08	-0.04
9.02	-	-	-	9.13	-0.11
11.01	-	-	-	11.06	-0.05
13.01	-	-	-	13.11	-0.10
15.01	-	-	-	15.07	-0.06
17.02	-	-	-	16.99	0.03
20.02	-	-	-	20.08	-0.06

Wind Aloft Plotting Board.	
US.DEPARTMENT OF COMMERCE WEATHER BUREAU	
WIND DIRETION	TESTED WIND DIRECTION
0	0
90	90
180	180
270	270

Calibrated by :

Wacharapol

Mr. Watcharapol Subwat

Mechanical Engineer

Calibration & Test Section
Meteorological Instruments Bureau



ภาคผนวก ง-2

ใบรับรองสอบเทียบเครื่องมือตรวจวัด
คุณภาพอากาศจากแหล่งกำเนิด



Environmental Solution Integrator Co., Ltd.

Web Site : www.esithailand.com

E-mail : info@esithailand.com

METHOD 5 CONSOLE CALIBRATION

USING REFERENCE WET TEST METER W-NK-2.5B No.545141


5-POINT METRIC UNIT

Meter Console Information	
Console Model Number	XC-572-V
Console Serial Number	0710060
DGM Model Number	SK25EX
DGM Serial Number	00006206

Calibration Conditions		
Date	Time	4-Mar-24
9:00 AM		
Calibration Reference No.	SE67AP004	
Barometric Pressure	760.00	mm Hg
Calibration Meter Gamma	1.010	

Factors/Conversions		
Std Temp	293	K
Std Press	760	mm Hg
K ₁	0.386	
Console Leak Check		
PASS		

Calibration Data									
Metering Console					Calibration Meter				
Run Time	DGM Orifice ΔH (P _m)	Volume Initial (V _{mi})	Volume Final (V _{mf})	Outlet Temp Initial (t _{mi})	Outlet Temp Final (t _{mf})	Volume Initial (V _{wi})	Volume Final (V _{wf})	Outlet Temp Initial (t _{wi})	Outlet Temp Final (t _{wf})
Elapsed (Θ)									
min	mm H ₂ O	m ³	m ³	°C	°C	m ³	m ³	°C	°C
11.50	13.0	1391.4824	1391.6224	24	24	554.833860	554.963000	22	22
11.93	13.0	1391.6224	1391.7624	24	24	554.963000	555.091660	22	22
8.00	26.0	1391.7694	1391.9094	24	25	555.097780	555.226960	22	22
8.03	26.0	1391.9094	1392.0494	25	25	555.226960	555.355680	22	22
13.10	40.0	1392.0560	1392.3360	25	25	555.360740	555.617940	22	22
13.05	40.0	1392.3360	1392.6160	25	25	555.617940	555.876100	22	21
11.73	50.0	1392.6362	1392.9162	25	26	555.893540	556.150560	21	21
11.60	50.0	1392.9162	1393.1962	26	26	556.150560	556.406540	21	21
9.70	70.0	1393.2030	1393.4830	26	26	556.412500	556.668460	21	21
9.67	70.0	1393.4830	1393.7630	26	26	556.668460	556.923000	21	21

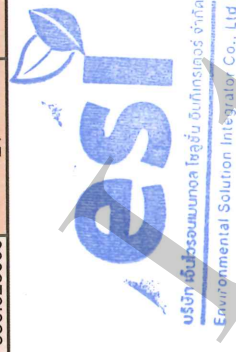



Environmental Solution Integrator Co., Ltd.

Web Site : www.esithailand.com

E-mail : info@esithailand.com

METHOD 5 CONSOLE CALIBRATION

USING REFERENCE WET TEST METER W-NK-2.5B No.545141

5-POINT METRIC UNIT

Calibration Data									
Results									
Standardized Data					Dry Gas Meter				
Dry Gas Meter		Calibration Meter		Calibration Factor		Flowrate		Variation	
($V_{m(sat)}$) m^3	($Q_{m(sat)}$) m^3/min	($V_{W(sat)}$) m^3	($Q_{W(sat)}$) m^3/min	Value (Y)	Variation (ΔY)	Std & Corr ($Q_{m(sat)(corr)}$) m^3/min	.0212 m^3_{ad}/min ($\Delta H@$) $mm\ H_2O$	Variation ($\Delta \Delta H@$)	
0.139	0.012	0.130	0.011	0.930	0.007	0.011	45.995	-0.137	
0.139	0.012	0.129	0.011	0.927	0.003	0.011	49.897	3.765	
0.139	0.017	0.130	0.016	0.930	0.006	0.016	44.601	-1.531	
0.139	0.017	0.129	0.016	0.926	0.003	0.016	45.296	-0.836	
0.279	0.021	0.258	0.020	0.924	0.001	0.020	46.539	0.407	
0.280	0.021	0.259	0.020	0.928	0.004	0.020	45.764	-0.368	
0.280	0.024	0.259	0.022	0.923	-0.001	0.022	46.666	0.534	
0.280	0.024	0.258	0.022	0.919	-0.005	0.022	45.983	-0.150	
0.281	0.029	0.258	0.027	0.917	-0.007	0.027	45.195	-0.937	
0.281	0.029	0.256	0.027	0.912	-0.012	0.027	45.387	-0.745	
Y Average				0.924			46.132	$\Delta H@$ Average	

esi
บริษัท เอสไอโซลูชันอินทิเกรเตอร์ จำกัด
Environmental Solution Integrator Co., Ltd.

Note: For Calibration Factor Y, the ratio of the reading of the calibration meter to the dry gas meter, acceptable tolerance of individual values from the average is ± 0.02 .
Note: For $\Delta H@$, orifice pressure differential that equates to 0.75cfm (0.0212 m^3/min) at standard temperature and pressure, acceptable tolerance of individual values from the average is ± 0.2 inches (5.1mm) H_2O .

Calibrated by : *Kiatkawan*


Approved by :

Terdong Samthong

Date

4-Mar-24


Meter Gamma vs Flowrate

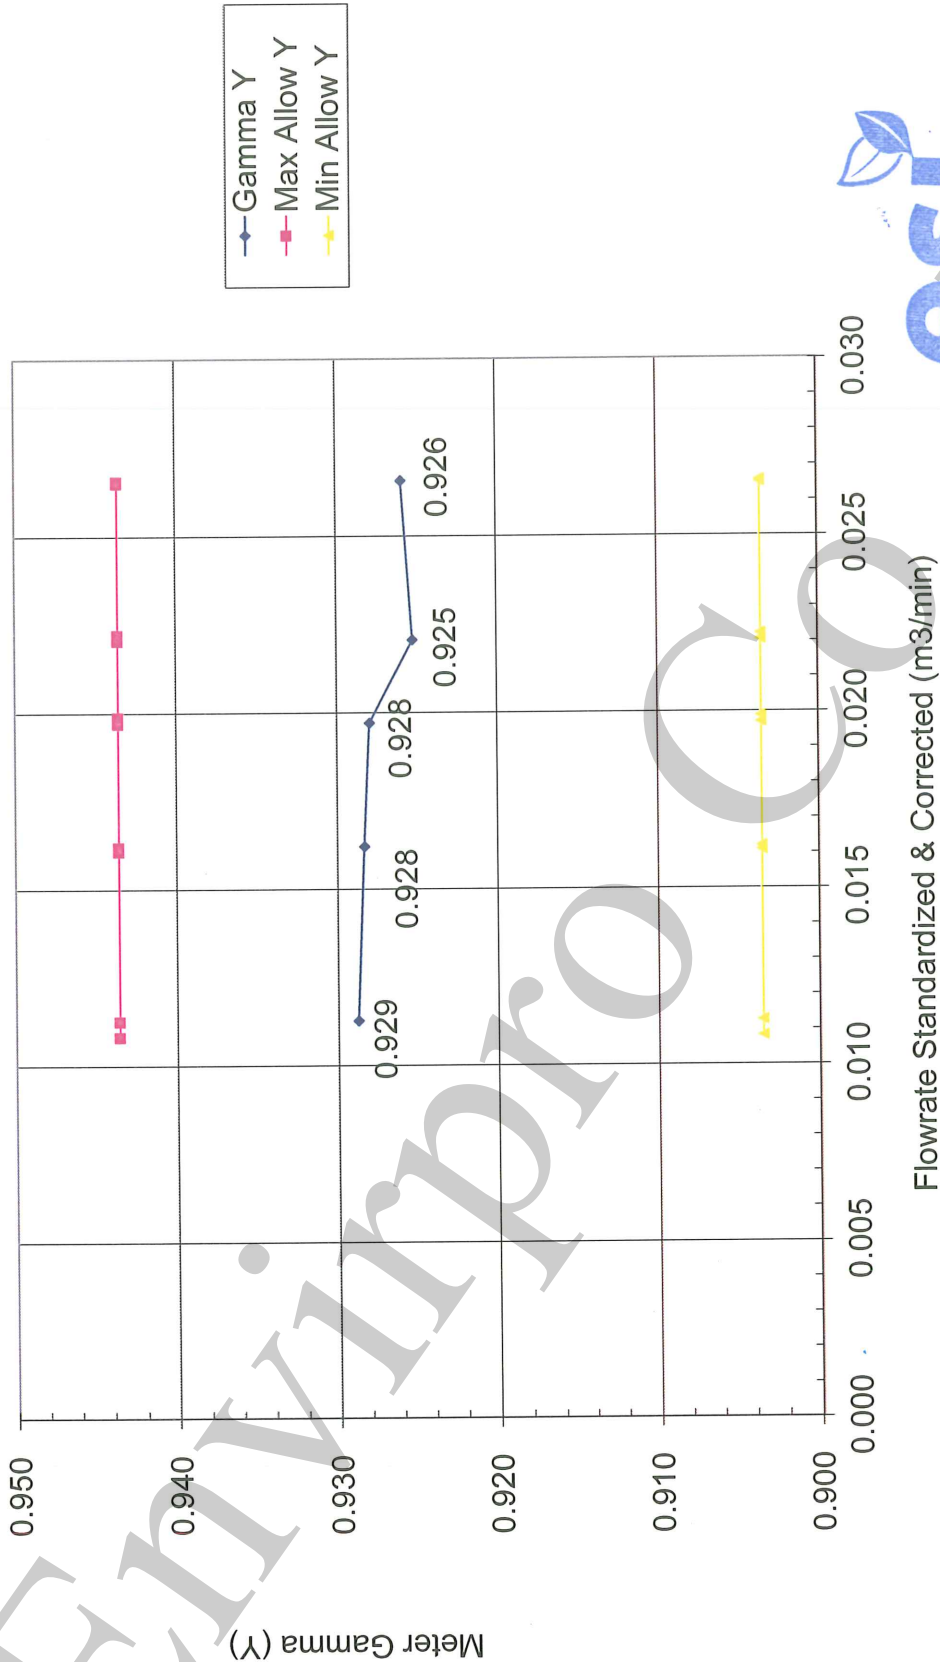

Console Serial: 0710060

Console Model: XC-572-V

Meter Pressure vs Flowrate

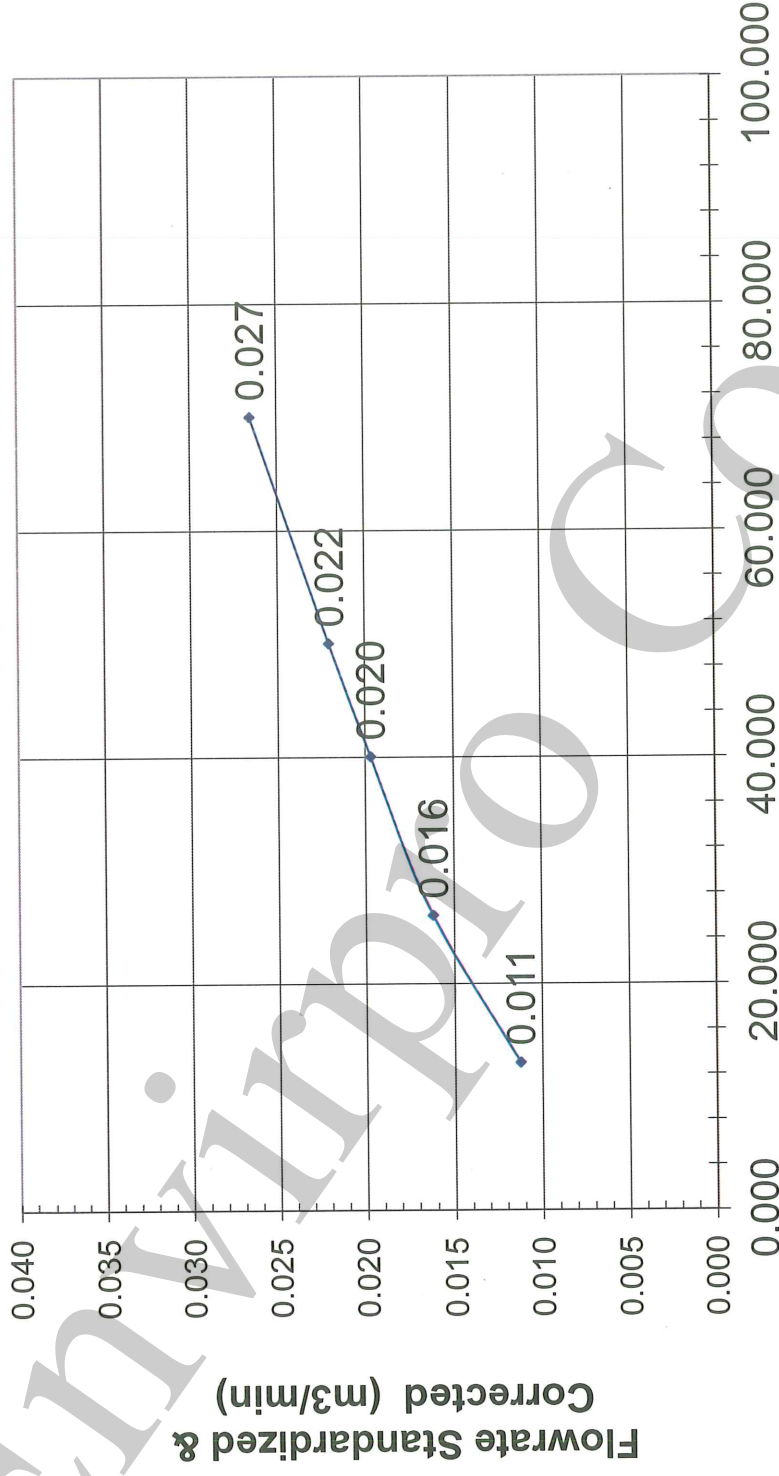



Environmental Solution Integrator Co., Ltd.
Web Site : www.esithailand.com
E-mail : info@esithailand.com

NOZZLE CALIBRATION

Sampling System Equipment Information		Calibration Conditions			
Console Model Number	XC-572-V	Date	SE67AP004	04-Mar-24	9:00 AM
Console Serial Number	0710060	Calibration Reference No.	SE67AP004		
DGM Model Number	SK25EX	Barometric Pressure	755	mm Hg	
DGM Serial Number	00006206	Calibration	Vernier ,0-150mm	0.01 mm increments	
Nozzle Types	Stainless	Method Reference	US.EPA Method		


Calibration Data					Results	
Nozzle ID	Nozzle Diameter				Different	$(D_1 + D_2 + D_3) / 3$
Sizes		D ₁	D ₂	D ₃	ΔD	Davg
	mm	mm	mm	mm	mm	mm
NS-4	3.2	2.90	2.89	2.91	0.010	2.900
NS-6	4.8	4.44	4.45	4.44	0.006	4.443
NS-8	6.4	6.12	6.12	6.13	0.006	6.123
NS-10	8.0	7.87	7.86	7.84	0.015	7.857
NS-12	9.5	9.53	9.51	9.52	0.010	9.520
NS-14	11.1	10.90	10.88	10.91	0.015	10.897
NS-16	12.7	12.73	12.71	12.74	0.015	12.727

Where :

D1, D2, D3 = There difference nozzle diameters , mm ; diameter must be within 0.025 mm

ΔD = Maximum difference between any two diameters, must be ≤ 0.100 mm

Davg = $(D_1 + D_2 + D_3) / 3$

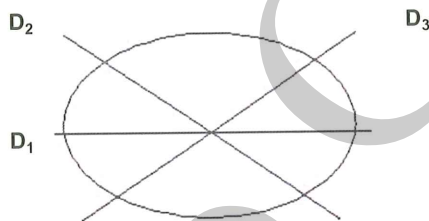

บริษัท เอ็นวิรอนเมนทอล โซลูชั่น อินทิเกรเตอร์ จำกัด
Environmental Solution Integrator Co., Ltd.

Calibrated by :

Kiatka win

Approved by :

Pasady Sangthong



Environmental Solution Integrator Co.,Ltd.
Web Site : www.esithailand.com
E-mail : info@esithailand.com

THERMOCOUPLES SYSTEM CALIBRATION

Samplig System Equipment Information

Console Model Number	XC-572-V
Console Serial Number	0710060
DGM Model Number	SK25EX
DGM Serial Number	00006206
Meter Box Model Number	JENCO 765
Meter Box Serial Number	JC17919

Calibration Conditions

Date	Time	04-Mar-24	10:30 AM
Calibration Reference No.	SE67AP004		
Reference Thermometer	FLUKE 714		
Serial Number	1812153		
Dry Box Calibrator	Pyros 650		
Serial Number	K38111		

Results

Console Thermocouple Simulator

Channal and test point	Meter Box Channal Temperature Reading (°C)											
	-18.0	25.0	38.0	93.0	149.0	260.0	371.0	482.0	593.0	816.0	1038.0	
Stack	-17	25	38	93	150	260	372	483	564	817	1038	
Aux	-17	25	38	93	150							
Probe	-17	25	38	93	150							
Filter	-17	25	38	93	150							
Exit	-17	25	38									

OUTLET DGM Thermocouple

Set Point	Reference Thermocouple	Probe Thermpcouple	Difference
30	30.0	29	0.33
40	40.0	38	0.64
50	50.0	48	0.62

Probe Thermocouple

Set Point	Reference Thermocouple	Probe Thermpcouple	Difference
100	100.0	98	0.54
250	250.0	246	0.76
300	300.0	298	0.35
350	350.0	347	0.48

Tolerances Range

Stack ± 1.50% Absolute
DGM ± 3.0 °C
Probe ± 3.0 °C

esi
Meter ± 3.0 °C
Filter ± 3.0 °C
Exit ± 2.0 °C
บริษัท เอสไอทีไทยแลนด์ จำกัด
Environmental Solution Integrator Co., Ltd.

Calibrated by : Kiatkawin

Approved by : Tanad' Sang Hong



Environmental Solution Integrator Co., Ltd.
Web Site : www.esithailand.com
E-mail : info@esithailand.com

PITOT TUBE CALIBRATION

Sampling System Equipment Information	
Console Model Number	XC-572-V
Console Serial Number	0710060
DGM Model Number	SK25EX
DGM Serial Number	00006206
Pitot tube Number	A10947

Calibration Conditions			
Date	3/4/2024	Time	05-Mar-24 9:00 AM
Calibration	SE67AP004	SE67AP004	
Barometric Pressure	759	mm Hg	
Pitot Tube Type	S		
size (OD)	3/8	inch	
Standard Pitot Tube ID Number	160-12		
C _p (std)	0.99		

Results				
"A" SIDE CALIBRATION				
RUN No.	Δp std	Δp (s)	C _p (s)	DEVIATION
	mm H ₂ O	mm H ₂ O		C _p (s)-C _p (A)
1	6.4	8.8	0.844	-0.005
2	16.4	22.2	0.851	0.001
3	30.8	41.4	0.854	0.004
	AVERAGE	C _p (SIDE A)	0.850	-0.003

Results				
"B" SIDE CALIBRATION				
RUN No.	Δp std	Δp (s)	C _p (s)	DEVIATION
	mm H ₂ O	mm H ₂ O		C _p (s)-C _p (B)
1	6.4	8.8	0.844	-0.003
2	16.4	22.4	0.847	-0.001
3	30.8	41.6	0.852	0.004
	AVERAGE	C _p (SIDE B)	0.848	-0.003

$$[C_p(\text{SIDE A}) - C_p(\text{SIDE B})] = 0.002 \quad (\text{must be } \leq 0.01)$$

Note: Average deviation must be < 0.01

บริษัท เอ็นวิรโพร เทคโนโลยี โซลูชั่น จำกัด
Environmental Solution Integrator Co., Ltd.

Calibrated by : Kiatkavin

Approved by : Terdang Samthong

CERTIFICATE OF CALIBRATION

Certificate No.: B1-0507031/24

Page 1 **of total** 4 **pages**

Customer ENVIRPRO CO., LTD.
168/28 Nakniwas Rd., Ladprao, Bangkok 10230

Equipment	Electronic Balance	Model	PL 1501-S
Manufacturer	METTLER TOLEDO	ID No.	SV-TL.081/2259
Serial No.	1203420225		
Description	Maximum Capacity: 1500 g	Resolution:	0.1 g

Environmental Conditions

Ambient Temperature:	24.9 °C
Relative Humidity:	62 %
Atmospheric Pressure:	-

Calibration Location Balance Room

Received Date 5 July 2024

Calibration Date 5 July 2024

Date of Issue 8 July 2024

Condition of Artifacts Used conditions but can be calibrated

Checked by



Act as Technical Manager

Approved by



Representative of Managing Director

<input type="checkbox"/> (Krisyosl K.)	<input type="checkbox"/> (Sakda Y.)
<input type="checkbox"/> (Patiphan K.)	<input type="checkbox"/> (Onnapa P.)
<input type="checkbox"/> (Pongsak H.)	<input type="checkbox"/> (Nitiphong K.)
<input checked="" type="checkbox"/> (Kanung C.)	<input type="checkbox"/> (Nonthachai K.)
<input type="checkbox"/> (Pramong P.)	<input type="checkbox"/> (Noppol P.)

(Dr. Ekachai Puttitwong)

Certificate No.: B1-0507031/24

Page 2 of total 4 pages

Reference Method:

- The calibration method used was CP-208 based on UKAS LAB 14
- This certificate can be traceable to the national standards, which is realized the shown measurement units according to the International System of Units (SI Units).

Reference Standard Instruments:

Type	Serial No.	Cert. No.	Due Date	Traceability
Standard Weight Set 1 mg - 5 kg	30402687-4	I0-2702002/23	Feb. 27, 2025	THC

Remark: This certificate is traceable to the International System of Unit (SI Unit) through:

- THC, Thai Heart Calibration Co., Ltd.

Measurement Results:

- ☒ Without Adjustment
☐ After Adjustment

1. Repeatability


Nominal Weight	Standard Deviation of Reading (g)
1300 g	0.00

Certificate No.: B1-0507031/24


Page 3 of total 4 pages

Measurement Results (Cont.):

2. Off-Center Loading



Front

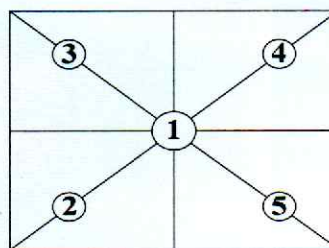

Front



Measuring Positions

Measuring Positions	Instrument Reading (g)	Max. Difference (g)
1	200.0	0.0
2	200.0	
3	200.0	
4	200.0	
5	200.0	
1	200.0	

3. Error of indication from nominal value

Standard Weight (g)	Instrument Reading (g)		Correction (g)	Uncertainty of Measurement (g)
	Without Adjustment	After Adjustment		
1.0	1.0	-	0.0	± 0.082
5.0	5.0	-	0.0	± 0.082
10.0	10.0	-	0.0	± 0.082
50.0	50.0	-	0.0	± 0.082
100.0	100.0	-	0.0	± 0.082
200.0	200.0	-	0.0	± 0.082
500.0	500.0	-	0.0	± 0.082
700.0	700.0	-	0.0	± 0.082
1000.0	1000.0	-	0.0	± 0.082
1200.0	1200.0	-	0.0	± 0.082
1300.0	1300.0	-	0.0	± 0.082

Calibrated by

Ariyaphon

Certificate No.: B1-0507031/24

Page 4 of total 4 pages

Measurement Results (Cont.):

4. Effect of Tare

Nominal Tare Weight (g)	Standard Weight (g)		Instrument Reading (g)	Instrument Deviation (g)
300	Tare		0.0	0.0
	at 20 %	200.0	200.0	0.0
	at 40 %	400.0	400.0	0.0
	at 60 %	600.0	600.0	0.0
	at 80 %	800.0	800.0	0.0
	at 100 %	1000.0	1000.0	0.0

The above reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor $k = 2.00$, providing a level of confidence approximately 95%.

- End of Certificate -

Certificate No: G 670258

Date of issue : 11-Apr-24

Instrument description : Flue Gas Analyzer
Instrument model : Testo 310
Control unit serial no. : -
Instrument serial no. : 42824262
ID no. or control no. : -
Manufacturer : Testo SE & Co. KGaA
Probe description : -
Probe model : -
Probe serial no. : -
Customer name : ENVIRPRO CO., LTD.
Customer address : 168/28 Nakniwas Rd, Ladprao, Bangkok 10230

Total pages of certificate : 2 Pages
Receiving no. : L-241458
Receiving date. : 11-Apr-24
Parameter of calibration : Gas Calibration(Oxygen 2.50,10.04,21.02 %vol, Carbon Monoxide 80.14,302,1003 ppm)

Condition of UUC. : Used
Ambient condition : All of the Measurment ware caried out the stabilized labotary
 Temperature : 23 ± 5 °C
 Humidity : 55 ± 15 %RH

Calibration place : 17/121 Soi Ngamwongwan 47 Yaek 48, Toongsonghong, Laksi, Bangkok 10210

Calibration procedure no. : This instrument was calibrated by comparison with Standard gas mixture according to calibration Work Instruction no. WI-CL-28-C

The calibration certificate expanded uncertainty of measurement is stated as the standard uncertainty of measurent Multiplied by coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

This certificate is applied only to item under test Environmental condition.

This Calibration Certificate may not be reporduced other than in full except with the permission of the issuing laboratory. Calibration certificates without signature and seal not valid and The results relate only to the items tested/calibrated.

This calibration certificate documents are tracebility to national standards, which realize measurement according to the International System of Units (SI).

Date of calibration : 11-Apr-24



Mr. Sedtawut Nueathong
Calibration Engineer



Mrs. Nongluck Wongsettee
Technical Manager

Certificate No.: G 670258

Standard References (Table 1)

Standard	Certificate No.	Vendor	Due date
Oxygen (O ₂) 2.50 % Vol	2412/23	Linde	27-Aug-27
Oxygen (O ₂) 10.04 % Vol	CG-0153-21	Nimt	18-Nov-26
Oxygen (O ₂) 21.02 % Vol	CG-0041-22	Nimt	10-Feb-27
Carbon monoxide (CO) 80.14 ppm	CG-0040-22	Nimt	14-Feb-27
Carbon monoxide (CO) 302 ppm	1915/23	Linde	16-Jun-25
Carbon monoxide (CO) 1003 ppm	2584/23	Linde	10-Sep-25

Measured room conditions

Temperature : 23.7 °C Humidity : 65.3 %RH Pressure : 1010.4 mbar

Calibration conditions

Gas Temperature : 24 °C Flow rate : 600 ml/min Gas pressure : 1013.7 mbar

Calibration Results (before adjustment) (Table 2)

Parameter of Standard	Standard Values	Mean of UUC	Error	Uncertainty (±)
O ₂ (%Vol)	2.50	2.5	0.00	0.15
O ₂ (%Vol)	10.04	10.0	-0.04	0.20
O ₂ (%Vol)	21.02	21.0	-0.02	0.30
CO (ppm)	80.14	76	-4.14	3.0
CO (ppm)	302	292	-10	6.0
CO (ppm)	1003	959	-44	12

Calibration Results (after adjustment) (Table 3)

Parameter of Standard	Standard Values	Mean of UUC	Error	Uncertainty (±)
O ₂ (%Vol)	2.50	2.5	0.00	0.15
O ₂ (%Vol)	10.04	10.0	-0.04	0.20
O ₂ (%Vol)	21.02	21.0	-0.02	0.30
CO (ppm)	80.14	79	-1.14	3.0
CO (ppm)	302	303	1	6.0
CO (ppm)	1003	1006	3	12

Remark : 1 cmol/mol = 1 %vol, 1 μmol/mol = 1 ppm.

End of Report



CALIBRATION LABORATORY Co., LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



CERTIFICATE OF CALIBRATION

FOR

NOMENCLATURE : BAROMETER
MANUFACTURER : BARIGO
MODEL / TYPE : N/A
SERIAL NO. : N/A[SV-TL.019/2550]
CLID. NO. : 212100899
JOB CONTROL NO. : 240803080226
CALIBRATION SERVICE : ☒ IN-LABORATORY ☐ ON-SITE

CUSTOMER : ENVIRPRO CO., LTD.
168/28 NAKNIWAS RD., LADPRAO,
BANGKOK 10230 THAILAND


DATE OF RECEIVED : 03 August 2024

DATE OF ISSUED : 06 August 2024

The report of calibration shall not be reproduced except in full without approval of the Calibration Laboratory Co., Ltd.

Calibrated By : Sittipong Pimdee
Calibration Engineer

Approved By : Mongkol Yotsoontorn
Authorized Signatory
06 August 2024



This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to the International System of Units (SI)

Certificate No. Q24080226

F3-011-05/12-23

page 1 of 3



@clccalibration

REPORT OF CALIBRATION

FOR

NOMENCLATURE : **BAROMETER**
MANUFACTURER : **BARIGO**
MODEL / TYPE : **N/A**
SERIAL NO. : **N/A[SV-TL.019/2550]**
DATE OF CALIBRATION : **05 August 2024**

ENVIRONMENT CONDITIONS :

Temperature : $(23 \pm 2) ^\circ\text{C}$

Relative Humidity : $(55 \pm 10) \% \text{RH}$

PROCEDURE USED :

This instrument was calibrated under procedure No. **CLC-CPPP-07** according to **DKD-R 6-1** as calibration guidelines.

The calibration was performed by direct measurement with Reference Pressure Monitor which maintained by the Calibration Laboratory Co., Ltd.

REFERENCE STANDARD USED :

Reference Pressure Monitor, Fluke Model RPM3 S/N. 829.

TRACEABILITY :

The measurements are traceable to International System of Units (SI), through National Institute of Metrology (Thailand).
Certificate No. MP-0229-23, Due Date 09 November 2024.

UNCERTAINTY :

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor of $k = 2$. It has been evaluated according to the " Calibration of Pressure Gauges (DKD-R 6-1)" which provides a level of confidence approximately 95%.

Certificate No. Q24080226

F3-011-05/12-23

page 2 of 3



CONDITION OF CALIBRATION ITEM : RECEIVED IN GOOD OPERATIONAL CONDITION

MEASUREMENT RESULTS : (X) without adjustment () adjustment

The DUC was exercised by applying a known pressure from its zero to full scale 1 times. Then 2 series of known gauge pressure were applied. The STD reading were recorded and the means value were reported in the table below.

CALIBRATION DATA

CORRECTION OF PRESSURE

DUC Test point (hPa)	STD Reading (hPa)		Correction (hPa)	
	Up	Down	Up	Down
970	970.9	970.9	+0.9	+0.9
980	980.7	980.8	+0.7	+0.8
990	990.6	990.7	+0.6	+0.7
1000	1000.4	1000.5	+0.4	+0.5
1010	1010.3	1010.4	+0.3	+0.4
1020	1020.2	1020.2	+0.2	+0.2
1030	1030.2	1030.2	+0.2	+0.2

Uncertainty of measurement ± 0.9 hPa

Transmitting fluid : Air.

Note. The Scope of Accredited ANAB Certificate No. ACDM-2814 Version 012 Page 44 of 67

This report is valid for the above stated instrument/s only.

End of Certificate

Certificate No. Q24080226

F3-011-05/12-23

page 3 of 3



@clccalibration

CERTIFICATE OF CALIBRATION

Certificate No. : 24-083917

Sample Code : 24-33404-005

Customer : บริษัท เอ็นไวโรโปร จำกัด
เลขที่ 168/28 ถนนนาคนิวาส แขวงลาดพร้าว
เขตลาดพร้าว กรุงเทพมหานคร 10230

Location of Calibration : Asia Medical and Agricultural Laboratory and Research Center Public Company Limited
(Calibration Laboratory)

Equipment : Cylinder

Manufacturer : witeg **Class** : A

Serial No. : N/A **ID No.** : SV-TL101/2562

Date of Receipt : 04 July 2024 **Date of Calibration** : 10 July 2024

Condition of Calibration

1. **Environment**
- 1.1 Ambient Temperature : $20^{\circ}\text{C} \pm 2.5^{\circ}\text{C}$
- 1.2 Atmospheric Pressure : $1013\text{ hPa} \pm 8\text{ hPa}$
- 1.3 Relative Humidity : $50\% \pm 10\%$
2. **Calibration method** : ASTM E542-01 (2012)
3. **Reference standard instrument**

Instrument	ID No.	Certificate No.	Due Date
3.1 Electronic Balance	LB-BL-10	23-083786	24 July 2024
3.2 Thermo Hygrometer	LB-DA-05	QR24-0509	04 March 2025
3.3 Barometer	LB-PS-04	23P4056	03 December 2024
3.4 Thermometer	LB-TH-34	23-098975	25 August 2024

4. This certificate is traceable to the international system of unit (SI Unit).

- 4.1 Instrument No. 3.1, 3.4 through : Asia Medical and Agricultural Laboratory and Research Center Public Company Limited
- 4.2 Instrument No. 3.2 through : Quality Reborn Co., Ltd.
- 4.3 Instrument No. 3.3 through : Technology Promotion Association (Thailand-Japan)

5. This result of calibration was found accurate as shown on date and place of calibration only.

6. **Condition of calibration item** : Normal

Calibrated by Miss Woranuch Sookruay
Scientist

Approved by (Mr. Somchai Neampunt)
Signed for Director

Issue date 18 July 2024

The uncertainties are for a confidence probability of approximately 95%.

The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Asia Medical and Agricultural Laboratory and Research Center Public Company Limited (AMARC).

NSC-TISI-TIS17025
CALIBRATION 0152

Page 2 of 2

REPORT OF CALIBRATION

Certificate No. : 24-083917

Sample Code : 24-33404-005

Equipment : Cylinder

Capacity : 1000 ml

Manufacturer : witeg

Class : A

Serial No. : N/A

ID No. : SV-TL.101/2562

Results of Calibration

Calibration results without adjustment.

The result obtained is the arithmetic average value of volumes from 10 single weighings.

SI Unit $\text{cm}^3 = \text{ml}$

Nominal value	(ml)	500	1000
Average reading	(ml)	500.63	1001.08
Standard deviation	(ml)	0.03	0.01
Error value	(ml)	-0.63	-1.08
Uncertainty	\pm (ml)	0.15	0.15
Coverage factor	(k)	2.00	2.00

The result expanded uncertainty of measurement U is stated as the standard uncertainty of measurement multiplied by the coverage factor k , which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty of measurement has been determined in accordance with UKAS M3003.

- End of Report -

Agilent CrossLab Start Up Services Agilent 7890 Gas Chromatograph Preventive Maintenance Checklist

Agilent Preventive Maintenance provides factory recommended service for your analytical instruments to assure reliable operation and the accuracy of your results.

Delivered by highly trained and certified service engineers using genuine Agilent parts and supplies, Agilent Preventive Maintenance provides everything you need to reduce unplanned downtime and keep your systems operating at their peak. This checklist will be completed at the end of the service and provided to you as a record of the preventive maintenance activities.



เอกสารไม่ควบคุม

Introduction

Customer Information

- Customers should provide all necessary operating supplies upon request of the engineer.
- A customer representative should be available to the engineer while performing the preventive maintenance procedures.
- Any parts, not included in the Parts Lists section of this document, are not part of the recommended Preventive Maintenance service, nor are they included in the price of this service.
- If a system requires the use of extra or special procedures and/or parts for the maintenance service, then these must be ordered separately and charged as a repair, which may incur additional costs.

Important Customer Web Links

- For more information about **Agilent Technologies services**, please visit our website using the following URL: <http://www.agilent.com/en-us/products/crosslab-instrument-services/service-repair>
- The **Agilent Community** is an excellent place to get answers, collaborate with others about applications and Agilent products, and find in-depth documents and videos relevant to Agilent technologies. Visit <https://community.agilent.com/welcome>.
- To access **Agilent University**, visit <http://www.agilent.com/crosslab/university/> to learn about training options, which include online, classroom and onsite delivery. A training specialist can work directly with you to help determine your best options.
- A useful **Agilent Resource Center** web page is available, which includes short videos on maintenance, quick lists of consumables for new instruments, and other valuable information. Check out the Resource Page here: <https://www.agilent.com/en-us/agilentresources>.
- Need technical support, FAQs, supplies? – visit our **Support Home page** <http://www.agilent.com/search/support>.
- **Videos** about specific preparation requirements for your instrument can be found by searching the **Agilent YouTube** channel at <https://www.youtube.com/user/agilent>.
- **7890B Manuals** are also available on Agilent.com:
 - **Safety**
https://www.agilent.com/cs/library/usermanuals/public/7890B_Safety.pdf
 - **Installation and First Startup**
https://www.agilent.com/cs/library/usermanuals/Public/7890B_Installation.pdf
 - **Operation Manual**
https://www.agilent.com/cs/library/usermanuals/Public/7890B_Operation.pdf
 - **Maintaining Your GC**
https://www.agilent.com/cs/library/usermanuals/public/G3430-90052%207890B_Maintaining%20Guide.pdf

Service Engineer's Responsibilities

- Contact the customer and ensure that all necessary supplies are available before the preventive maintenance visit.
- Only select those pages that relate to the system or module being serviced.
- Complete empty fields with the relevant information.
- Complete the relevant checkboxes in the checklist using either a "X" or tick mark "✓".
- Check "**Section not applicable**" check boxes to indicate services/tasks not delivered, as appropriate.
- Complete the Preventive Maintenance service in the order of the tasks listed.
- Complete the Service Review section together with the customer.
- Complete the fields for page numbers at the foot of each selected page
- Complete the total number of pages field in the Service Completion section
- **Ask the customer to sign the Service Completion section including the customer's and your signature.**

Additional Instruction Notes

- Check for any active service notes for this unit. If there are any applicable "Safety" or "Modification Recommended" Service notes, plan to implement the changes on this unit before doing any qualification service.
- Do not implement firmware updates, unless you get approval from the customer and are sure that they are compatible with the instrument control software.

System Information

- ☒ Check this box if an instrument configuration report is attached instead of completing the table below.

Instrument System Name and ID	CN11021007
Instrument System Site and Location	Instrument Room

List System Component Product Numbers	List the Serial Numbers of each Component
1. G3440A	CN11021007
2.	
3.	
4.	
5.	
6.	
7.	
8.	
9.	
10.	

Preparation

- ☒ Discuss any specific issues with the customer before starting.
- ☒ Review the instrument logbook for recorded problems and comments.
- ☒ Save instrument control settings before starting the procedure.
- ☒ Perform a general inspection of the system for cleanliness.
- ☒ Check for proper installation of parts, assemblies, sensors etc.
- ☒ Check system for required installation of components, settings as defined by current Service Notes.
- ☒ Check for required firmware updates and verify with customers if they would like them installed.
- ☒ Before starting the following procedures, record the Detector Signal Output(s) in the results table. If the GC is turned OFF or in a service mode, comparing the detector outputs before and after the service is not possible.

Revision: 2.00, Issued: December 30, 2020
Agilent Document Number: D0007063
DE number: 44166.7597222222
© Agilent Technologies, Inc. 2020

Page 4 of 9



เอกสารไม่ควบคุม

Preventive Maintenance Procedure

Clean and inspect GC

- ☒ Unplug power cord from the power source.
- ☒ Open GC covers and vacuum/remove any dust/debris. Pay particular attention to cooling fans.
- ☒ Inspect internal connectors for proper contact and placement.
- ☒ Reconnect Power to the GC. Power the GC on and verify the power on self-test passed.
- ☒ Verify oven motor spins freely and turns on with the oven door closed; off when the door is opened.
- ☒ Verify operation of all other fans - the inlet and EPC cooling fans.
- ☒ Verify oven intake/outlet flap assembly is operating smoothly while heating and cooling the oven

Inlet and detector consumable replacement

- ☒ For the inlets installed, perform inlet maintenance as defined in the 7890 manual – “Maintaining Your GC” - for the inlet(s) installed.
- ☒ Replace the split vent trap cartridge filter on units with these inlets: Split/Splitless Capillary (SSL), Multi-Mode Inlet (MMI), Programmed Temperature Vaporizer (PTV), Volatiles Interface (VI).
- ☒ If the inlet system is used in Split Mode with viscous samples, inspect and clean the split vent tube on the inlet and flush or replace the tubing between the inlet and the split vent trap.
- ☒ If the GC includes a Flame Ionization Detector (FID), replace the jet. If the ignitor shows any buildup of sample or corrosion, replace the ignitor. Examine the FID collector and castle assemblies for contamination – clean as necessary.

Zero Sensors and Leak test

- ☒ Zero all pressure sensors per the procedure in the 7890 “Advanced User Guide”.
- ☒ Perform inlet pressure decay test(s) as defined in the 7890 “Troubleshooting Manual”.
If the PM is done in preparation for an Operational Qualification, then the pressure decay test defined within that protocol can be used for the PM.
- ☒ Record if test passed or failed in the results table.

ALS Maintenance

- ☐ **Section NOT applicable**
- ☒ Check all cabling and configuration settings between GC, tray, and injectors.
- ☒ Vacuum or remove any dust, especially around fans.
- ☒ Check operation of all fans.
- ☒ Check syringe for smooth plunger operation.
- ☒ Check for smooth operation of the needle support – clean if necessary

Restore Instrument

- ☒ Restore the normal operating conditions or customer method using the Browser interface or Data System.
- ☒ Purge the system with carrier flow for 15 minutes
- ☒ Bake out the system, then restore the normal operating conditions
- ☒ After equilibration, check and record the post PM detector signal output values. Results should be similar or lower than the detector outputs recorded prior to PM.
- ☒ Perform a chemical checkout. If this is a routine PM, inject the customer's sample using the ALS if applicable. This will act as a final checkout of both the ALS and the GC.

Note: If the PM Service is performed prior to a qualification service, then use the qualification procedure as a guide for final instrument set up and checkout.

Signature Page

Service Review

- ☒ Attach available reports/printouts of all tests to this documentation.
- ☒ Record the Preventive Maintenance service activity in the customer's records/logbook.
- ☒ Update/reset instrument maintenance counters as appropriate.
- ☒ Affix the PM sticker to the system or instrument logbook based on the customer's request.
- ☒ Complete the Service Engineer Comments section if there are additional comments.
- ☒ Review with the customer this service, parts replaced, and test results obtained.
- ☒ If the instrument firmware was updated, record the details of the change in the Service Engineer's Comments box or if necessary, in the customer's IQ records.
- ☐ Supply the customer with a copy of the Smart Alerts flyer.
- ☐ Describe Smart Alerts to the customer.
- ☐ Install Smart Alerts if requested.

7890 GC Test Results Table

Detector Signal Outputs	Before PM Service	After PM Service
Front detector output	NA.	NA.
Back detector output	NA.	22.0
AUX detector output	NA.	NA.
Pressure decay test	Expected test result	Actual test result
Front inlet pressure decay test	Pass	Pass
Back inlet pressure decay test	Pass	NA.

7890 Parts List Table

The following kits are recommended for capillary and purged packed inlets. If this is a general PM and the customer has a preferred set of consumables, you may use the customer's consumables.

Part description	Part number	Product or model# where used	Quantity consumed
SSL Capillary Inlet PM kit, Splitless	5188-6497	7890A/B	1
SSL Capillary Inlet PM kit, split	5188-6496	7890A/B	
SSL Capillary Ultra Inert Inlet Gold Seal with Washer	5190-6144	7890A/B	
SSL Capillary Ultra Inert Inlet Splitless Liner - Single taper with Glass Wool	5190-2293	7890A/B	
SSL Capillary Ultra Inert Inlet Low Pressure Drop Split Liner - with Glass Wool	5190-2295	7890A/B	
PP Inlet PM kit	5188-6498	7890A/B	
Split vent trap PM kit, single cartridge (for MMI, PTV & VI)	5188-6495	7890A/B	
MMI Cleaning Kit	G3510-60820	7890A/B	
PTV Septumless Head Rebuild Kit	5182-9747	7890A/B	
PTV Septumless Head Teflon Guide	5182-9748	7890A/B	
Ignitor (glow plug) assembly with O-ring	19231-60680	7890A/B	1
FID Collector Rebuild/Cleaning Kit	G1531-67000	7890A/B	
Standard .011-inch FID Jet for capillary FID base	G1531-80560	7890A/B	1
High Temperature .018-inch FID Jet for capillary FID base	G1531-80620	7890A/B	
Standard .018-inch FID Jet for packed column with packed FID base	18710-20119	7890A/B	
Standard .011-inch FID Jet for capillary column with packed/adaptable FID base	19244-80560	7890A/B	
High Temperature .018-inch FID Jet for capillary column with packed/adaptable FID base	19244-80620	7890A/B	
NPD Jet, universal fit, .011-inch ID	G1534-80580	7890A/B	
NPD Jet, universal fit, .011-inch ID Extended tip	G1534-80590	7890A/B	
SSL Capillary Ultra Inert Inlet Gold Seal with Washer	5190-6144	7890A/B	
SSL Capillary Ultra Inert Inlet Splitless Liner - Single taper with Glass Wool	5190-2293	7890A/B	
**FID Collector Replacement Kit, if needed	G1531-67001	7890A/B	

Revision: 2.00, Issued: December 30, 2020
 Agile Document Number: D0007063
 DE number: 44166.759722222
 © Agilent Technologies, Inc. 2020

Page 8 of 9



เอกสารไม่ควบคุม

Service Engineer Comments

If there are any specific points you wish to note as part of performing the service or other items of interest for the customer, please write include them in this box.

Service Completion

Service request number 6006748380 Date service completed 21Feb2024
Agilent signature Phuwanai Yoktragul Customer signature _____
Total number of pages in this document 9

ภาคผนวก ง-3

ใบรับรองสอบเทียบเครื่องมือตรวจวัดระดับเสียงทั่วไป

CERTIFICATE OF CALIBRATION

Certificate No.: E0-1907003/24

Page 1 **of total** 2 **pages**

Customer ENVIRPRO CO., LTD.
168/28 Nakniwas Rd., Ladprao, Bangkok 10230

Equipment	Sound Calibrator		
Manufacturer	TENMARS	Model	TM-100
Serial No.	210502635	ID No.	-
Description	-		

Environmental Conditions Ambient Temperature: $(23 \pm 3) ^\circ\text{C}$
Relative Humidity: $(50 \pm 15) \%$
Atmospheric Pressure: -

Calibration Location Wildcats Laboratory (EL)

Received Date 19 July 2024

Calibration Date 20 July 2024

Date of Issue 22 July 2024


Condition of Artifacts Used conditions but can be calibrated

Checked by



Act as Technical Manager

Approved by

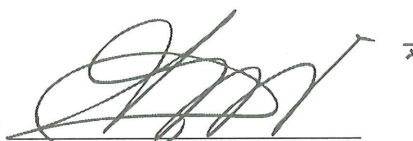

Representative of Managing Director

() (Krisyosl K.)	() (Sakda Y.)
(✓) (Patiphan K.)	() (Onnapa P.)
() (Pongsak H.)	() (Nitiphong K.)
() (Kanung C.)	() (Nonthachai K.)
() (Pramong P.)	() (Noppol P.)

(Dr. Ekachai Puttitwong)

Certificate No.: E0-1907003/24

Page 2 of total 2 pages

Reference Method:

- The calibration method used was based on in-house method.
- This certificate can be traceable to the national standards, which is realized the shown measurement units according to the International System of Units (SI Units).

Reference Standard Instruments:

Type	Serial No.	Cert. No.	Due Date	Traceability
Sound Level Calibrator	Z130263	CP20230421EA	Dec. 25, 2024	EEI
Digital Sound Level Meter	040208595	CP20240015EA	Dec. 24, 2024	EEI

Remark: This certificate is traceable to the International System of Unit (SI Unit) through:

- EEI, Electrical and Electronics Institute, Foundation for Industrial Development.

Measurement Results:

Sound Accuracy Test.

UUC Applied	Measured Value	Error	Uncertainty \pm
94.0 dB	94.0 dB	0.0 dB	0.3 dB
114.0 dB	114.0 dB	0.0 dB	0.3 dB

UUC : Unit Under Calibration

The above reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor $k = 2.00$, providing a level of confidence approximately 95%.

- End of Certificate -

Calibrated by Jakkarin

Certificate of Calibration

Certificate No.: C2312-0580

Customer: ENVIRPRO COMPANY LIMITED
168/28 Nakniwas Road,
Ladprao, Bangkok 10230

Date of calibration: 2023-12-25
Date of issue: 2023-12-25
Instrument Calibrated: Sound Calibrator
Manufacturer: TENMARS
Type: ST-120
Serial no: 211203744

Calibration and verification performed:

The performed tests refer to IEC 60942 (2017): Electroacoustics - Sound Calibrators. The calibrator has been tested as described in Annex B of the same standard.

Preconditioning:

The equipment was preconditioned for more than 16 hours at the specified calibration temperature and humidity

Instruments and Program:

A complete list of instruments, hardware, and software, that has been used for this calibration is separately available from the calibration laboratory.

Equipment standards used:

- Sound Measuring Equipment Calibration Unit 483B S/N31083
- Digital Multimeter Keysight S/N HP34401A
- Ultra-low Distortion Function Generator Stanford SRS DS360 S/N123625
- Acoustic Sound Calibrator Class 0 Nor1253 S/N32941
- Reference Microphone Condenser G.R.A.S. 40AU-1 S/N309231
- Sound Analyser Nor140 S/N1405248
- System Software Nor1504A

Traceability

The measured values are traceable to following the ISO/IEC 17025 laboratories:

Sound Pressure Level: NCL, Norway

Reference Microphone: NCL, Norway

Voltage: TPA, Thailand

Frequency: TPA, Thailand

Distortion Meter: EEI, Thailand

This certificate of calibration is issued by Acoustic Laboratory Thailand (ALT). It also states that the laboratory has a satisfactory quality assurance system and traceability to accredited or national calibration laboratories. This certificate may not be reproduced other than in full.

Environmental conditions:	Pressure:	Temperature:	Relative humidity:
Reference conditions:	101.325 kPa	23.0 °C	50 %RH
Measurement conditions:	101.93 ± 0.02 kPa	22.8 ± 1.2 °C	53.9 ± 2.9 %RH

1. Sound pressure level

Specified sound pressure level (dB)	Measured sound pressure level (dB)	Deviated value (dB)	Tolerance limit IEC60942:2017 Class 1 (dB)
Reference microphone 40AU S/N 309231			
94.00	94.96	0.96	±0.25
114.00	115.12	1.12	±0.25

2. Frequency

Specified Frequency (Hz)	Measured Frequency (Hz)	Deviated value (%)	Tolerance limit IEC60942:2017 Class 1 (%)
Reference microphone 40AU S/N 309231			
1000.00	999.96	0.00	±0.7
1000.00	999.96	0.00	±0.7

3. Total distortion + Noise

Specified sound pressure level (dB)	Measured Distortion (%)	Tolerance limit IEC60942:2017 Class 1 (%)
94.00	0.3	±2.5
114.00	2.7	±2.5

Uncertainty of measurement

Parameters	Uncertainty
Sound pressure level	0.10 dB
Frequency	0.020 %
Total distortion + Noise	0.10 %

Date of calibration: 2023-12-25

Date of issue : 2023-12-25

Certificate No.: C2312-0580

The reported expanded uncertainty is based upon a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

Calibrated By:
(Mr. Athakom sumphan)

Approved By:
(Mr. Pitupong Sarapho)

Date of calibration: 2023-12-25

Date of issue : 2023-12-25

----- End of Certificate of Calibration -----

ภาคผนวก ง-4

ใบรับรองสอบเทียบเครื่องมือตรวจวัดคุณภาพอากาศ
ในสถานประกอบการ

Certificate of Calibration

Customer

Name : ENVIRPRO CO., LTD.
Address : 168/28 Nakniwas Rd., Ladprao, Bangkok 10230

Certificate No : 23-AFM-256

Request No : Req-2023-2405

Unit Under Calibration Details

Measurement Item : Air Flow Meter

Manufacturer : MesaLabs

Model : Defender 510

Sensor Model : -

Serial Number : 205593

Sensor Serial Number : -

ID : -

Location of Calibration : LAB 4 AIR VELOCITY METER

Calibration Environment and Details

Temperature : 23 °C ± 3 °C

Humidity : 55 %RH ± 20 %RH

Barometric Pressure : 1013 hPa ± 10 hPa

Received Date : 10 November 2023

Calibration Date : 19 December 2023

Calibration Procedure : In-house method CP-AFM-01 by Comparison technique with Standard Primary Flow Calibrator

Reference Standard	Model	Serial Number	Traceble	Due Calibration
Air Flow Meter	Gilibrator 3 Low flow	18501010006	Sensidyne	12 July 2024
Air Flow Meter	Gilibrator 3 Standard flow	19031011003	Sensidyne	12 July 2024
Temperature meter	GT 11	08000057	Qreborn	27 February 2024
Pressure meter	CPG2400	41000KDU/651882	TPA	7 November 2023


Traceability :

This Certificate is traceable to SI Unit through Sensidyne A2LA Accreditation No. 3943.01


Note :

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor $k = 2$, providing a level of confidence approximately 95 %.

Calibration By :


Mr. Noppadon Luangart
Service Calibration Engineer

Approved By :


Mr. Pacit Mathavorn
Calibration Engineer Supervisor

Issue Date : 19 December 2023

Certificate No : 23-AFM-256

Request No : Req-2023-2405

Result of Calibration :

Temperature (°C)	Pressure (kPa)	STD (l/min)	UUC (l/min)	Error (l/min)	Uncertainty (l/min)
25.00	101.20	0.501	0.50129	0.0003	0.0077
25.20	101.20	1.005	1.0059	0.001	0.015
25.30	101.10	2.006	2.0049	-0.001	0.028
25.40	101.00	3.006	3.0083	0.002	0.043
25.40	100.80	5.047	5.0449	-0.002	0.073

Note

STD : Standard UUC : Unit Under Calibration

- UUC Reference Condition : At atmospheric pressure and room temperature condition

- Flow Rate was corrected for non-standard operating condition by using equation :

$$Q_{meas} = Q_{ref} \times \frac{P_{ref}}{P_{meas}} \times \frac{T_{meas}}{T_{ref}}$$

where Q = Flow Rate P = Absolute Pressure T = Absolute Temperature

Meas = Measurement Condition ref = Standard Condition

* Indicates non accredited

End of Certificate

CERTIFICATE OF CALIBRATION

Certificate No.: B1-2602013/24

Page 1 **of total** 5 **pages**

Customer ENVIRPRO CO., LTD.
168/28 Nakniwas Rd., Ladprao, Bangkok 10230

Equipment Electronic Balance

Manufacturer AND

Model HR-202i

Serial No. 15204549

ID No. SV-TL.121/2565

Description Maximum Capacity: 50 g

Resolution: 0.00001 g

Maximum Capacity: 220 g

Resolution: 0.0001 g

Environmental Conditions Ambient Temperature: 27.1 °C

Relative Humidity: 42.5 %

Atmospheric Pressure: -

Calibration Location ห้องเครื่องชั่ง

Received Date 26 February 2024

Calibration Date 26 February 2024

Date of Issue 27 February 2024

Condition of Artifacts Used conditions but can be calibrated

Checked by



Act as Technical Manager

Approved by



Representative of Managing Director

- | | |
|---|--|
| <input type="checkbox"/> (Krisyosl K.) | <input type="checkbox"/> (Sakda Y.) |
| <input type="checkbox"/> (Patiphan K.) | <input type="checkbox"/> (Onnapa P.) |
| <input type="checkbox"/> (Pongsak H.) | <input type="checkbox"/> (Nitiphong K.) |
| <input checked="" type="checkbox"/> (Kanung C.) | <input type="checkbox"/> (Nonthachai K.) |
| <input type="checkbox"/> (Pramong P.) | <input type="checkbox"/> (Noppol P.) |

(Dr. Ekachai Puttitwong)

This calibration certificate shall not be reproduced other than in full except with the prior written approval of the Thai Heart Calibration Co., Ltd.

Certificate No.: B1-2602013/24

Page 2 of total 5 pages

Reference Method:

- The calibration method used was CP-208 based on UKAS LAB 14
- This certificate can be traceable to the national standards, which is realized the shown measurement units according to the International System of Units (SI Units).

Reference Standard Instruments:

Type	Model	Serial No.	Cert. No.	Due Date	Traceability
Standard Weight Set 1 mg - 200 g	-	158841	MM-0032-22	Mar. 15, 2024	NIMT

Remark: This certificate is traceable to the International System of Unit (SI Unit) through:

- NIMT, National Institute of Metrology (Thailand).

Measurement Results:

- ☒ Without Adjustment
☐ After Adjustment

1. Repeatability


Nominal Weight	Standard Deviation of Reading (g)
200 g	0.00003

Certificate No.: B1-2602013/24


Page 3 of total 5 pages

Measurement Results (Cont.):

2. Off-Center Loading



Front

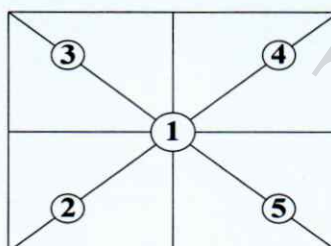

Front



Measuring Positions

Measuring Positions	Instrument Reading (g)	Max. Difference (g)
1	49.99996	0.00012
2	50.00002	
3	49.99994	
4	49.99990	
5	50.00002	
1	49.99997	

3. Error of indication from nominal value

Standard Weight (g)	Instrument Reading (g)		Correction (g)	Uncertainty of Measurement (g)
	Without Adjustment	After Adjustment		
0.00100	0.00099	-	0.00001	± 0.000043
0.00300	0.00300	-	0.00000	± 0.000044
0.00500	0.00501	-	-0.00001	± 0.000043
0.01000	0.01002	-	-0.00002	± 0.000044
0.05000	0.05002	-	-0.00002	± 0.000044
0.10000	0.10001	-	-0.00001	± 0.000044
0.50000	0.50001	-	-0.00001	± 0.000045
1.00000	1.00000	-	0.00000	± 0.000045
9.99998	9.99999	-	-0.00001	± 0.000052
19.99997	20.00001	-	-0.00004	± 0.000062
29.99995	30.00002	-	-0.00007	± 0.000074
40.00000	40.00007	-	-0.00007	± 0.000074

Calibrated by

Natthapong

Certificate No.: B1-2602013/24

Page 4 of total 5 pages

Measurement Results (Cont.):

3.Error of indication from nominal value (Cont.)

Standard Weight (g)	Instrument Reading (g)		Correction (g)	Uncertainty of Measurement (g)
	Without Adjustment	After Adjustment		
49.99993	49.99997	-	-0.00004	± 0.000081
59.9999	60.0000	-	-0.0001	± 0.00014
69.9999	70.0000	-	-0.0001	± 0.00014
79.9999	80.0000	-	-0.0001	± 0.00014
84.9999	85.0000	-	-0.0001	± 0.00014
89.9999	89.9999	-	0.0000	± 0.00015
99.9999	99.9998	-	0.0001	± 0.00016
109.9999	109.9999	-	0.0000	± 0.00028
119.9999	119.9999	-	0.0000	± 0.00028
129.9998	130.0000	-	-0.0002	± 0.00028
139.9999	140.0000	-	-0.0001	± 0.00028
149.9998	150.0000	-	-0.0002	± 0.00028
159.9998	160.0000	-	-0.0002	± 0.00028
169.9998	170.0000	-	-0.0002	± 0.00028
179.9998	180.0000	-	-0.0002	± 0.00028
189.9998	190.0000	-	-0.0002	± 0.00028
199.9999	200.0000	-	-0.0001	± 0.00028

Calibrated by Natthapong

Certificate No.: B1-2602013/24

Page 5 of total 5 pages

Measurement Results (Cont.):

4. Effect of Tare

Nominal Tare Weight (g)	Standard Weight (g)		Instrument Reading (g)	Instrument Deviation (g)
50	Tare		0.0000	0.0000
	at 20 %	10.0000	10.0000	0.0000
	at 40 %	20.0000	20.0001	0.0001
	at 60 %	50.0000	49.9998	-0.0002
	at 80 %	100.0000	100.0000	0.0000
	at 100 %	150.0000	150.0000	0.0000

The above reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor $k = 2.00$, providing a level of confidence approximately 95%.

- End of Certificate -

GC Clarus 500/580 Preventive Maintenance (PM)

Company Name:			
Address (Instrument Location):			
Serial Number:		Service Tag:	
Customer Name (if applicable):		PM number:	
Service Engineer Name:		Service Order Number:	
Date PM Performed: (DD-MMM-YYYY)		Next PM Due Date: (DD-MMM-YYYY)	

Part Number	Release	Publication Date	
TH09370050	2.2	Jan 2020	

Scope

The purpose of this PM is to ensure the continued functionality of the Clarus 500 and Clarus 580 GC by inspecting and replacing any worn or damaged parts. This service should only be performed by a trained representative of PerkinElmer. The customer should save their method before the PM begins.

General Instructions:

The customer must provide the engineer operational data to demonstrate recent instrument performance prior to starting the PM. Always check with the customer before making any changes that may affect the customer's analysis or calibration, including a current back-up of system software and/or data files. The completed document should be signed by an authorized PerkinElmer and customer representative and left with the customer. Update the PM sticker and instrument logbook as required.

Copyright Information

This document contains proprietary information that is protected by copyright. All rights are reserved. No part of this publication may be reproduced in any form whatsoever or translated into any language without the prior, written permission of Perkin Elmer, Inc. **Copyright © 2013 PerkinElmer, Inc.**

Trademarks

Registered names, trademarks, etc. used in this document, even when not specifically marked as such, are protected by law. PerkinElmer is a registered trademark of PerkinElmer, Inc. All other trademarks and registered trademarks not owned by PerkinElmer, Inc. or its subsidiaries that are depicted herein are the property of their respective owners. **Except as specifically set forth in its terms and conditions of sale, PerkinElmer makes no Warranty of any kind with regard to this document, including, but not limited to, the implied warranties of merchantability and fitness for a particular purpose.** PerkinElmer shall not be liable for incidental or consequential damages in connection with the furnishing or use of this document.

Component List

Component / Specific Model	Serial #	Software Version	Configuration Notes

Parts Lists

Additional Tools Required for PM				
Part Number (if applicable)	Description	Quantity	Serial #	Calibration Due Date (MM/YY)
Additional Reagents and Standards Required for PM				
Part Number (if applicable)	Description	Quantity	Batch/Lot #	Expiration Date (MM/YY)

Procedure Checklist

Use (✓) to check off those steps in the checklist that have been completed.

1. General:

Review the instrument performance with the customer and document any recent problems.

Check incoming AC line voltage for proper levels and grounding.

L-N _____ Volt
L-G _____ Volt
N-G _____ Volt

**Neutral to ground not more than 0.5 volts peak to peak*

Inspect all gas line filters and traps; Replace if necessary with customer supplied spares.

Carrier gas	Helium	Nitrogen	Hydrogen	
Moisture level	Good	Need to replace	Other	_____
Detector gas	Air Zero	Hydrogen	Nitrogen	Helium
Moisture level	Good	Need to replace	Other	_____

Inspect the customer log book and make any appropriate PM entries.

Leak check all fittings from the gas source to instrument.

Gas leakage Pass Fail Comment _____

Perform general inspection of system for cleanliness.

Inspect for functional and clean electronic cooling and oven vent fans

Electronic cooling fan	Yes	No
Oven cooling fan	Yes	No

2. Electronic :

Check oven temperature. Calibrate if necessary.

Oven temperature set point °C Pass Fail

Check sub-ambient option. (If installed).

Oven temperature set point 5 °C Pass Fail

Perform routine maintenance on detector/injector. Replace parts as necessary with customer supplied spares.

Check flows, including split flows if applicable. Calibrate if necessary.

Carrier flow Pass Fail

Split flow

Check detector gas flows and adjust if necessary.

Detector flow Pass Fail

Autosampler installed Yes No

Check autosampler sensor for wear and replace if necessary.

Vial sensor Pass Fail

Door sensor Pass Fail

Tower sensor Pass Fail

Plunger sensor Pass Fail

Elevator sensor Pass Fail

Remove syringe, manually flush. Replace with customer supplied spare if necessary.

Check firmware version. Upgrade to current levels if necessary.

Firmware version _____

Measure all accessible power supply voltages.

5 Volt Pass Fail

+15 Volt Pass Fail

-15 Volt Pass Fail

24 Volt Pass Fail

Record all detector voltage signal.

Detector Channel A _____ mV.

Detector Channel B _____ mV.

3. Diagnostics Tests:

Run instrument diagnostics.

BRAM Pass Fail

EPROM Pass Fail

Run Autosampler diagnostics.

BRAM Pass Fail

EPROM Pass Fail

4. Review:

Review with the customer PM work performed.

Review with the customer routine maintenance procedures.

Discuss recommended customer-supplied materials to have on hand

Attach PM sticker.

Update Logbook.

Additional Comments

Additional Comments Regarding the PM

Review

<p><i>The preventive maintenance checks and if applicable performance tests for Clarus500/580 GC have been completed.</i></p>	
<p><i>This Clarus500/580 GC</i></p>	<p><i>the preventive maintenance.</i></p>
<p>Review of Preventive Maintenance:</p>	
<p>Authorized PerkinElmer Representative:</p> <p><i>Nisan</i></p>	<p>Date:</p> <p>(DD-MMM-YYYY)</p>
<p>Authorized Customer Representative:</p> <p><i>Wank</i></p>	<p>Date:</p> <p>(DD-MMM-YYYY)</p>

Service Report

Work Order Number	Activity Code	Billing Type	Requested Start Date	Model	Serial Number
WO-02928942	Repair	Contract	25/07/2567 10:11 น.	CLARUS500	650N3022702
Service Representative Name	Contract Number	Expiry Date	Equipment ID	System ID	
Inkum, Wisan	SC-0035622058	13/06/2025	N/A	N/A	
UDI Number					
N/A					
Equipment Location			Bill To Name		
บริษัท เอ็นไวร์โปร จำกัด เขตลาดพร้าว กรุงเทพฯ 51 10230 TH			บริษัท เอ็นไวร์โปร จำกัด เขตลาดพร้าว กรุงเทพมหานคร 51 10230 TH		
Customer Contact	Phone Number	Fax Number	Email	Purchase Order	
K. Sasitron	0-2831-6699	0-2831-6698	N/A	6501023	

Work Description		
PM1/2 replace PM kit. add N6101183 Auto sample vial locator spring. 09902143 Silicone rubber O-ring Check flows, including split flows. Check detector gas flows Check Oven temperature Check autosampler sensor Remove syringe, manually flush. Replace with customer supplied spare if necessary. Measure all accessible power supply voltages.		
Start Date	End Date	Work Description
25/07/2024	25/07/2024	
25/07/2024	25/07/2024	
31/07/2024	31/07/2024	
31/07/2024	31/07/2024	

Tools Used					
Quantity	Calibrated Tool	Description	Serial Number	Last Calibration Date	Next Calibration Date
*** No Calibrated Tools Used ***					

Material Used				
Part Number	Part Description	Note	Lot/Serial Number	Quantity
N6101182	Replacement Vial Locator for Autosampler			1
N6121004	Quartz Liner for Spit Operation; 2 mm ID			1
09921004	O-Ring 9.32 OD x 5.32 ID			1
N6001204	Jet Contact Spring for External Igniter			1
N6100432	PIN ASSY-ASXL FID POL			1
N9306873	Blue GC Inlet Septa 10 Pk			1

Labour Details			
Part Number	Part Description	Start Date	Quantity
SV000013	Preventative maintenance	25/07/2024	4
SV000004	Service F.O.C. Travel	25/07/2024	1
SV000013	Preventative maintenance	31/07/2024	2
SV000004	Service F.O.C. Travel	31/07/2024	1

Work Complete		Customer Signature	Technician Signature
Yes	<input checked="" type="checkbox"/>	No	<input type="checkbox"/>
PM/OQ/IPV Left with Customer		 31/7/2567 K. Sasitron	 31/7/2567 Inkum, Wisan
Yes	<input type="checkbox"/>		

Terms & Conditions
<p>Customer Acknowledgment of receipt of the above repair / replacement.</p> <p>Special Terms and Conditions: This is not an invoice.</p> <p>Taxes will be applied to your invoice if applicable.</p>



ID LINE : IEC17025



Certificate of Calibration

Certificate Number : SPR24070076-2

Page : 1 of 3

Customer : ENVIRPRO CO.,LTD.

168/28 Nakniwas Road., Ladprao, Ladprao, Bangkok 10230

Equipment Name : Sound Level Meter

Manufacturer : ACO

Model : 6236

Serial Number : 222223

ID. Number : N/A

Environmental Conditions

Ambient Temperature : 23 °C \pm 3 °C

Received Date : 03 Jul 2024

Relative Humidity : 50 % \pm 15 %

Calibration Date : 04 Jul 2024

Location of Calibration : In-Lab

Recommend Due Date : N/A

Calibration Procedure : SP-CPE-04-01

Date of Issue : 05 Jul 2024

Method of Calibration

This certifies that the above instrument was calibrated in compliance with the calibration system requirement of ISO/IEC 17025:2017 in accordance with reference procedure. Standards used to perform this calibration are certified by to NIST or equivalent, National metrology institute, Natural physical constants, consensus standards. The result reported herein apply only to the calibration of the item described above as received. Our decision rule is to contact the customer if the item pass and fail calibration when the results include the uncertainties and the customer must determine if the results meets their needs.

The calibration certificate shall not be reproduced except in full, without written approval of SP Metrology System (Thailand).

Calibrated by : Mr.Nanthawat Wanasit

Calibration Officer

Approved by :

(Mr.Prayoon Topart)

Authorized Signatory



ID LINE : IEC17025



Calibration Report

Certificate Number : SPR24070076-2

Page : 2 of 3

Reference Standards

Equipment Name	Model	Serial No.	Certificate No.	Due. Date
Sound Level Calibrator	ST-120	211203773	EEL.BP. 140/0167	26 Jan 2025

Traceability

This certification is traceable to the International System of Unit maintained at :
TISTR - Thailand Institute of Scientific and Technological Research



ID LINE : IEC17025



Result of Calibration

Certificate Number : SPR24070076-2

Page : 3 of 3

Range : 94 to 114 dB

Function : @1kHz

Select A

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.0	94.0	0.0	0.0	0.15
114	113.9	113.9	-0.1	-0.1	0.15

Select C

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	93.9	93.9	-0.1	-0.1	0.15
114	113.8	113.8	-0.2	-0.2	0.15

Select Z

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	93.9	93.9	-0.1	-0.1	0.15
114	113.8	113.8	-0.2	-0.2	0.15

Note :

The result of calibration was found accurate as show on date and place of calibration only.
This Certificate is not certified for any commercial transaction.

Measurement Uncertainty

The reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor $k = 2.00$, providing a level of confidence approximately 95%.

- End of Certificate -



ID LINE : IEC17025



Certificate of Calibration

Certificate Number : SPR24070076-6

Page : 1 of 3

Customer : ENVIRPRO CO.,LTD.

168/28 Nakniwas Road., Ladprao, Ladprao, Bangkok 10230

Equipment Name : Sound Level Meter

Manufacturer : ACO

Model : 6236

Serial Number : 222224

ID. Number : N/A

Environmental Conditions

Ambient Temperature : 23 °C \pm 3 °C

Received Date : 03 Jul 2024

Relative Humidity : 50 % \pm 15 %

Calibration Date : 04 Jul 2024

Location of Calibration : In-Lab

Recommend Due Date : N/A

Calibration Procedure : SP-CPE-04-01

Date of Issue : 05 Jul 2024

Method of Calibration


This certifies that the above instrument was calibrated in compliance with the calibration system requirement of ISO/IEC 17025:2017 in accordance with reference procedure. Standards used to perform this calibration are certified by to NIST or equivalent, National metrology institute, Natural physical constants, consensus standards. The result reported herein apply only to the calibration of the item described above as received. Our decision rule is to contact the customer if the item pass and fail calibration when the results include the uncertainties and the customer must determine if the results meets their needs.

The calibration certificate shall not be reproduced except in full, without written approval of SP Metrology System (Thailand).

Calibrated by : Mr.Nanthawat Wanasit

Calibration Officer

Approved by :


(Mr.Prayoon Topart)

Authorized Signatory



ID LINE : IEC17025



Calibration Report

Certificate Number : SPR24070076-6

Page : 2 of 3

Reference Standards

Equipment Name	Model	Serial No.	Certificate No.	Due. Date
Sound Level Calibrator	ST-120	211203773	EEL.BP. 140/0167	26 Jan 2025

Traceability

This certification is traceable to the International System of Unit maintained at :
TISTR - Thailand Institute of Scientific and Technological Research



ID LINE : IEC17025



Result of Calibration

Certificate Number : SPR24070076-6

Page : 3 of 3

Range : 94 to 114 dB

Function : @1kHz

Select A

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.0	94.0	0.0	0.0	0.15
114	113.9	113.9	-0.1	-0.1	0.15

Select C

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	93.9	93.9	-0.1	-0.1	0.15
114	113.8	113.8	-0.2	-0.2	0.15

Select Z

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	93.9	93.9	-0.1	-0.1	0.15
114	113.8	113.8	-0.2	-0.2	0.15

Note :

The result of calibration was found accurate as show on date and place of calibration only.
This Certificate is not certified for any commercial transaction.

Measurement Uncertainty

The reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor $k = 2.00$, providing a level of confidence approximately 95%.

- End of Certificate -



ID LINE : IEC17025



Certificate of Calibration

Certificate Number : SPR24070076-8

Page : 1 of 3

Customer : ENVIRPRO CO.,LTD.

168/28 Nakniwas Road., Ladprao, Ladprao, Bangkok 10230

Equipment Name : Sound Level Meter

Manufacturer : ACO

Model : 6236

Serial Number : 222225

ID. Number : N/A

Environmental Conditions

Ambient Temperature : 23 °C \pm 3 °C

Received Date : 03 Jul 2024

Relative Humidity : 50 % \pm 15 %

Calibration Date : 04 Jul 2024

Location of Calibration : In-Lab

Recommend Due Date : N/A

Calibration Procedure : SP-CPE-04-01

Date of Issue : 05 Jul 2024

Method of Calibration


This certifies that the above instrument was calibrated in compliance with the calibration system requirement of ISO/IEC 17025:2017 in accordance with reference procedure. Standards used to perform this calibration are certified by to NIST or equivalent, National metrology institute, Natural physical constants, consensus standards. The result reported herein apply only to the calibration of the item described above as received. Our decision rule is to contact the customer if the item pass and fail calibration when the results include the uncertainties and the customer must determine if the results meets their needs.

The calibration certificate shall not be reproduced except in full, without written approval of SP Metrology System (Thailand).

Calibrated by : Mr.Nanthawat Wanasit

Calibration Officer

Approved by :


(Mr.Prayoon Topart)

Authorized Signatory



ID LINE : IEC17025



Calibration Report

Certificate Number : SPR24070076-8

Page : 2 of 3

Reference Standards

Equipment Name	Model	Serial No.	Certificate No.	Due. Date
Sound Level Calibrator	ST-120	211203773	EEL.BP. 140/0167	26 Jan 2025

Traceability

This certification is traceable to the International System of Unit maintained at :
TISTR - Thailand Institute of Scientific and Technological Research



ID LINE : IEC17025



Result of Calibration

Certificate Number : SPR24070076-8

Page : 3 of 3

Range : 94 to 114 dB

Function : @1kHz

Select A

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.0	94.0	0.0	0.0	0.15
114	113.9	113.9	-0.1	-0.1	0.15

Select C

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	93.9	93.9	-0.1	-0.1	0.15
114	113.8	113.8	-0.2	-0.2	0.15

Select Z

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	93.9	93.9	-0.1	-0.1	0.15
114	113.8	113.8	-0.2	-0.2	0.15

Note :

The result of calibration was found accurate as show on date and place of calibration only.
This Certificate is not certified for any commercial transaction.

Measurement Uncertainty

The reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor $k = 2.00$, providing a level of confidence approximately 95%.

- End of Certificate -



ID LINE : IEC17025



Certificate of Calibration

Certificate Number : SPR24070076-4

Page : 1 of 3

Customer : ENVIRPRO CO.,LTD.

168/28 Nakniwas Road., Ladprao, Ladprao, Bangkok 10230

Equipment Name : Sound Level Meter

Manufacturer : ACO

Model : 6236

Serial Number : 222226

ID. Number : N/A

Environmental Conditions

Ambient Temperature : 23 °C \pm 3 °C

Received Date : 03 Jul 2024

Relative Humidity : 50 % \pm 15 %

Calibration Date : 04 Jul 2024

Location of Calibration : In-Lab

Recommend Due Date : N/A

Calibration Procedure : SP-CPE-04-01

Date of Issue : 05 Jul 2024

Method of Calibration


This certifies that the above instrument was calibrated in compliance with the calibration system requirement of ISO/IEC 17025:2017 in accordance with reference procedure. Standards used to perform this calibration are certified by to NIST or equivalent, National metrology institute, Natural physical constants, consensus standards. The result reported herein apply only to the calibration of the item described above as received. Our decision rule is to contact the customer if the item pass and fail calibration when the results include the uncertainties and the customer must determine if the results meets their needs.

The calibration certificate shall not be reproduced except in full, without written approval of SP Metrology System (Thailand).

Calibrated by : Mr.Nanthawat Wanasit

Calibration Officer

Approved by :


(Mr.Prayoon Topart)

Authorized Signatory



ID LINE : IEC17025



Calibration Report

Certificate Number : SPR24070076-4

Page : 2 of 3

Reference Standards

Equipment Name	Model	Serial No.	Certificate No.	Due. Date
Sound Level Calibrator	ST-120	211203773	EEL.BP. 140/0167	26 Jan 2025

Traceability

This certification is traceable to the International System of Unit maintained at :
TISTR - Thailand Institute of Scientific and Technological Research





ID LINE : IEC17025



Certificate of Calibration

Certificate Number : SPR24070076-7

Page : 1 of 3

Customer : ENVIRPRO CO.,LTD.

168/28 Nakniwas Road., Ladprao, Ladprao, Bangkok 10230

Equipment Name : Sound Level Meter

Manufacturer : ACO

Model : 6236

Serial Number : 222227

ID. Number : N/A

Environmental Conditions

Ambient Temperature : 23 °C \pm 3 °C

Received Date : 03 Jul 2024

Relative Humidity : 50 % \pm 15 %

Calibration Date : 04 Jul 2024

Location of Calibration : In-Lab

Recommend Due Date : N/A

Calibration Procedure : SP-CPE-04-01

Date of Issue : 05 Jul 2024

Method of Calibration

This certifies that the above instrument was calibrated in compliance with the calibration system requirement of ISO/IEC 17025:2017 in accordance with reference procedure. Standards used to perform this calibration are certified by to NIST or equivalent, National metrology institute, Natural physical constants, consensus standards. The result reported herein apply only to the calibration of the item described above as received. Our decision rule is to contact the customer if the item pass and fail calibration when the results include the uncertainties and the customer must determine if the results meets their needs.

The calibration certificate shall not be reproduced except in full, without written approval of SP Metrology System (Thailand).

Calibrated by : Mr.Nanthawat Wanasit

Calibration Officer

Approved by :

(Mr. Prayoon Topart)

Authorized Signatory



ID LINE : IEC17025



Calibration Report

Certificate Number : SPR24070076-7

Page : 2 of 3

Reference Standards

Equipment Name	Model	Serial No.	Certificate No.	Due. Date
Sound Level Calibrator	ST-120	211203773	EEL.BP. 140/0167	26 Jan 2025

Traceability

This certification is traceable to the International System of Unit maintained at :
TISTR - Thailand Institute of Scientific and Technological Research



ID LINE : IEC17025



Result of Calibration

Certificate Number : SPR24070076-7

Page : 3 of 3

Range : 94 to 114 dB

Function : @1kHz

Select A

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.0	94.0	0.0	0.0	0.15
114	113.9	113.9	-0.1	-0.1	0.15

Select C

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	93.9	93.9	-0.1	-0.1	0.15
114	113.9	113.9	-0.1	-0.1	0.15

Select Z

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	93.9	93.9	-0.1	-0.1	0.15
114	113.8	113.8	-0.2	-0.2	0.15

Note :

The result of calibration was found accurate as show on date and place of calibration only.
This Certificate is not certified for any commercial transaction.

Measurement Uncertainty

The reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor $k = 2.00$, providing a level of confidence approximately 95%.

- End of Certificate -



ID LINE : IEC17025



Certificate of Calibration

Certificate Number : SPR24070076-1

Page : 1 of 3

Customer : ENVIRPRO CO.,LTD.

168/28 Nakniwas Road., Ladprao, Ladprao, Bangkok 10230

Equipment Name : Sound Level Meter

Manufacturer : ACO

Model : 6236

Serial Number : 222228

ID. Number : N/A

Environmental Conditions

Ambient Temperature : 23 °C \pm 3 °C

Received Date : 03 Jul 2024

Relative Humidity : 50 % \pm 15 %

Calibration Date : 04 Jul 2024

Location of Calibration : In-Lab

Recommend Due Date : N/A

Calibration Procedure : SP-CPE-04-01

Date of Issue : 05 Jul 2024

Method of Calibration

This certifies that the above instrument was calibrated in compliance with the calibration system requirement of ISO/IEC 17025:2017 in accordance with reference procedure. Standards used to perform this calibration are certified by to NIST or equivalent, National metrology institute, Natural physical constants, consensus standards. The result reported herein apply only to the calibration of the item described above as received. Our decision rule is to contact the customer if the item pass and fail calibration when the results include the uncertainties and the customer must determine if the results meets their needs.

The calibration certificate shall not be reproduced except in full, without written approval of SP Metrology System (Thailand).

Calibrated by : Mr.Nanthawat Wanasit

Calibration Officer

Approved by :

(Mr.Prayoon Topart)

Authorized Signatory



ID LINE : IEC17025



Calibration Report

Certificate Number : SPR24070076-1

Page : 2 of 3

Reference Standards

Equipment Name	Model	Serial No.	Certificate No.	Due. Date
Sound Level Calibrator	ST-120	211203773	EEL.BP. 140/0167	26 Jan 2025

Traceability

This certification is traceable to the International System of Unit maintained at :

TISTR - Thailand Institute of Scientific and Technological Research



ID LINE : IEC17025



Result of Calibration

Certificate Number : SPR24070076-1

Page : 3 of 3

Range : 94 to 114 dB

Function : @1kHz

Select A

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.0	94.0	0.0	0.0	0.15
114	113.9	113.9	-0.1	-0.1	0.15

Select C

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	93.9	93.9	-0.1	-0.1	0.15
114	113.8	113.8	-0.2	-0.2	0.15

Select Z

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	93.9	93.9	-0.1	-0.1	0.15
114	113.8	113.8	-0.2	-0.2	0.15

Note :

The result of calibration was found accurate as show on date and place of calibration only.
This Certificate is not certified for any commercial transaction.

Measurement Uncertainty

The reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor $k = 2.00$, providing a level of confidence approximately 95%.

- End of Certificate -



ID LINE : IEC17025



Certificate of Calibration

Certificate Number : SPR24070076-9

Page : 1 of 3

Customer : ENVIRPRO CO.,LTD.

168/28 Nakniwas Road., Ladprao, Ladprao, Bangkok 10230

Equipment Name : Sound Level Meter

Manufacturer : ACO

Model : 6236

Serial Number : 222229

ID. Number : N/A

Environmental Conditions

Ambient Temperature : $23^{\circ}\text{C} \pm 3^{\circ}\text{C}$

Received Date : 03 Jul 2024

Relative Humidity : $50\% \pm 15\%$

Calibration Date : 04 Jul 2024

Location of Calibration : In-Lab

Recommend Due Date : N/A

Calibration Procedure : SP-CPE-04-01

Date of Issue : 05 Jul 2024

Method of Calibration

This certifies that the above instrument was calibrated in compliance with the calibration system requirement of ISO/IEC 17025:2017 in accordance with reference procedure. Standards used to perform this calibration are certified by to NIST or equivalent, National metrology institute, Natural physical constants, consensus standards. The result reported herein apply only to the calibration of the item described above as received. Our decision rule is to contact the customer if the item pass and fail calibration when the results include the uncertainties and the customer must determine if the results meets their needs.

The calibration certificate shall not be reproduced except in full, without written approval of SP Metrology System (Thailand).

Calibrated by : Mr.Nanthawat Wanasit

Calibration Officer

Approved by :

(Mr. Prayoon Topart)

Authorized Signatory



ID LINE : IEC17025



Calibration Report

Certificate Number : SPR24070076-9

Page : 2 of 3

Reference Standards

Equipment Name	Model	Serial No.	Certificate No.	Due. Date
Sound Level Calibrator	ST-120	211203773	EEL.BP. 140/0167	26 Jan 2025

Traceability

This certification is traceable to the International System of Unit maintained at :
TISTR - Thailand Institute of Scientific and Technological Research



ID LINE : IEC17025



Result of Calibration

Certificate Number : SPR24070076-9

Page : 3 of 3

Range : 94 to 114 dB

Function : @1kHz

Select A

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.0	94.0	0.0	0.0	0.15
114	113.9	113.9	-0.1	-0.1	0.15

Select C

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	93.8	93.8	-0.2	-0.2	0.15
114	113.9	113.9	-0.1	-0.1	0.15

Select Z

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	93.9	93.9	-0.1	-0.1	0.15
114	113.9	113.9	-0.1	-0.1	0.15

Note :

The result of calibration was found accurate as show on date and place of calibration only.
This Certificate is not certified for any commercial transaction.

Measurement Uncertainty

The reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor $k = 2.00$, providing a level of confidence approximately 95%.

- End of Certificate -



ID LINE : IEC17025



Certificate of Calibration

Certificate Number : SPR24070076-12

Page : 1 of 3

Customer : ENVIRPRO CO.,LTD.

168/28 Nakniwas Road., Ladprao, Ladprao, Bangkok 10230

Equipment Name : Sound Level Meter

Manufacturer : ACO

Model : 6236

Serial Number : 222230

ID. Number : N/A

Environmental Conditions

Ambient Temperature : 23 °C \pm 3 °C

Received Date : 03 Jul 2024

Relative Humidity : 50 % \pm 15 %

Calibration Date : 04 Jul 2024

Location of Calibration : In-Lab

Recommend Due Date : N/A

Calibration Procedure : SP-CPE-04-01

Date of Issue : 05 Jul 2024

Method of Calibration

This certifies that the above instrument was calibrated in compliance with the calibration system requirement of ISO/IEC 17025:2017 in accordance with reference procedure. Standards used to perform this calibration are certified by to NIST or equivalent, National metrology institute, Natural physical constants, consensus standards. The result reported herein apply only to the calibration of the item described above as received. Our decision rule is to contact the customer if the item pass and fail calibration when the results include the uncertainties and the customer must determine if the results meets their needs.

The calibration certificate shall not be reproduced except in full, without written approval of SP Metrology System (Thailand).

Calibrated by : Mr.Nanthawat Wanasit

Calibration Officer

Approved by :

(Mr.Prayoon Topart)

Authorized Signatory



ID LINE : IEC17025



Calibration Report

Certificate Number : SPR24070076-12

Page : 2 of 3

Reference Standards

Equipment Name	Model	Serial No.	Certificate No.	Due, Date
Sound Level Calibrator	ST-120	211203773	EEL.BP. 140/0167	26 Jan 2025

Traceability

This certification is traceable to the International System of Unit maintained at :

TISTR - Thailand Institute of Scientific and Technological Research



ID LINE : IEC17025



Result of Calibration

Certificate Number : SPR24070076-12

Page : 3 of 3

Range : 94 to 114 dB

Function : @1kHz

Select A

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.0	94.0	0.0	0.0	0.15
114	114.0	114.0	0.0	0.0	0.15

Select C

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	93.9	93.9	-0.1	-0.1	0.15
114	113.9	113.9	-0.1	-0.1	0.15

Select Z

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	93.9	93.9	-0.1	-0.1	0.15
114	113.9	113.9	-0.1	-0.1	0.15

Note :

The result of calibration was found accurate as show on date and place of calibration only.
This Certificate is not certified for any commercial transaction.

Measurement Uncertainty

The reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor $k = 2.00$, providing a level of confidence approximately 95%.

- End of Certificate -



ID LINE : IEC17025



Certificate of Calibration

Certificate Number : SPR24070076-10

Page : 1 of 3

Customer : ENVIRPRO CO.,LTD.

168/28 Nakniwas Road., Ladprao, Ladprao, Bangkok 10230

Equipment Name : Sound Level Meter

Manufacturer : ACO

Model : 6236

Serial Number : 222231

ID. Number : N/A

Environmental Conditions

Ambient Temperature : $23^{\circ}\text{C} \pm 3^{\circ}\text{C}$

Received Date : 03 Jul 2024

Relative Humidity : $50\% \pm 15\%$

Calibration Date : 04 Jul 2024

Location of Calibration : In-Lab

Recommend Due Date : N/A

Calibration Procedure : SP-CPE-04-01

Date of Issue : 05 Jul 2024

Method of Calibration


This certifies that the above instrument was calibrated in compliance with the calibration system requirement of ISO/IEC 17025:2017 in accordance with reference procedure. Standards used to perform this calibration are certified by to NIST or equivalent, National metrology institute, Natural physical constants, consensus standards. The result reported herein apply only to the calibration of the item described above as received. Our decision rule is to contact the customer if the item pass and fail calibration when the results include the uncertainties and the customer must determine if the results meets their needs.

The calibration certificate shall not be reproduced except in full, without written approval of SP Metrology System (Thailand).

Calibrated by : Mr.Nanthawat Wanasit

Calibration Officer

Approved by :


(Mr.Prayoon Topart)

Authorized Signatory



ID LINE : IEC17025



Calibration Report

Certificate Number : SPR24070076-10

Page : 2 of 3

Reference Standards


Equipment Name	Model	Serial No.	Certificate No.	Due. Date
Sound Level Calibrator	ST-120	211203773	EEL.BP. 140/0167	26 Jan 2025

Traceability

This certification is traceable to the International System of Unit maintained at :
TISTR - Thailand Institute of Scientific and Technological Research



ID LINE : IEC17025



Result of Calibration

Certificate Number : SPR24070076-10

Page : 3 of 3

Range : 94 to 114 dB

Function : @1kHz

Select A

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.0	94.0	0.0	0.0	0.15
114	114.0	114.0	0.0	0.0	0.15

Select C

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	93.9	93.9	-0.1	-0.1	0.15
114	113.9	113.9	-0.1	-0.1	0.15

Select Z

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	93.9	93.9	-0.1	-0.1	0.15
114	113.9	113.9	-0.1	-0.1	0.15

Note :

The result of calibration was found accurate as show on date and place of calibration only.
This Certificate is not certified for any commercial transaction.

Measurement Uncertainty

The reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor $k = 2.00$, providing a level of confidence approximately 95%.

- End of Certificate -



ID LINE : IEC17025



Certificate of Calibration

Certificate Number : SPR24070076-11

Page : 1 of 3

Customer : ENVIRPRO CO.,LTD.

168/28 Nakniwas Road., Ladprao, Ladprao, Bangkok 10230

Equipment Name : Sound Level Meter

Manufacturer : ACO

Model : 6236

Serial Number : 222232

ID. Number : N/A

Environmental Conditions

Ambient Temperature : 23 °C \pm 3 °C

Received Date : 03 Jul 2024

Relative Humidity : 50 % \pm 15 %

Calibration Date : 04 Jul 2024

Location of Calibration : In-Lab

Recommend Due Date : N/A

Calibration Procedure : SP-CPE-04-01

Date of Issue : 05 Jul 2024

Method of Calibration

This certifies that the above instrument was calibrated in compliance with the calibration system requirement of ISO/IEC 17025:2017 in accordance with reference procedure. Standards used to perform this calibration are certified by to NIST or equivalent, National metrology institute, Natural physical constants, consensus standards. The result reported herein apply only to the calibration of the item described above as received. Our decision rule is to contact the customer if the item pass and fail calibration when the results include the uncertainties and the customer must determine if the results meets their needs.

The calibration certificate shall not be reproduced except in full, without written approval of SP Metrology System (Thailand).

Calibrated by : Mr.Nanthawat Wanasit

Calibration Officer

Approved by :

(Mr.Prayoon Topart)

Authorized Signatory



ID LINE : IEC17025



Calibration Report

Certificate Number : SPR24070076-11

Page : 2 of 3

Reference Standards

Equipment Name	Model	Serial No.	Certificate No.	Due, Date
Sound Level Calibrator	ST-120	211203773	EEL.BP. 140/0167	26 Jan 2025

Traceability

This certification is traceable to the International System of Unit maintained at :

TISTR - Thailand Institute of Scientific and Technological Research



ID LINE : IEC17025



Result of Calibration

Certificate Number : SPR24070076-11

Page : 3 of 3

Range : 94 to 114 dB

Function : @1kHz

Select A

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.0	94.0	0.0	0.0	0.15
114	114.0	114.0	0.0	0.0	0.15

Select C

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	93.9	93.9	-0.1	-0.1	0.15
114	113.9	113.9	-0.1	-0.1	0.15

Select Z

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	93.9	93.9	-0.1	-0.1	0.15
114	113.8	113.8	-0.2	-0.2	0.15

Note :

The result of calibration was found accurate as show on date and place of calibration only.
This Certificate is not certified for any commercial transaction.

Measurement Uncertainty

The reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor $k = 2.00$, providing a level of confidence approximately 95%.

- End of Certificate -



ID LINE : IEC17025



Certificate of Calibration

Certificate Number : SPR24030065-3

Page : 1 of 3

Customer : ENVIRPRO CO.,LTD.

168/28 Nakniwas Road., Ladprao, Ladprao, Bangkok 10230

Equipment Name : Noise Dosimeter

Manufacturer : Quest Technologies

Model : Q-400

Serial Number : QDA080044

ID. Number : N/A

Environmental Conditions

Ambient Temperature : $23^{\circ}\text{C} \pm 3^{\circ}\text{C}$

Received Date : 06 Mar 2024

Relative Humidity : $50\% \pm 15\%$

Calibration Date : 09 Mar 2024

Location of Calibration : In-Lab

Recommend Due Date : N/A

Calibration Procedure : SP-CPE-04-01

Date of Issue : 10 Mar 2024

Method of Calibration

This certifies that the above instrument was calibrated in compliance with the calibration system requirement of ISO/IEC 17025:2017 in accordance with reference procedure. Standards used to perform this calibration are certified by to NIST or equivalent, National metrology institute, Natural physical constants, consensus standards. The result reported herein apply only to the calibration of the item described above as received. Our decision rule is to contact the customer if the item pass and fail calibration when the results include the uncertainties and the customer must determine if the results meets their needs.

The calibration certificate shall not be reproduced except in full, without written approval of SP Metrology System (Thailand).

Calibrated by : Mr.Chumpon Dokpikul

Calibration Officer

Approved by :

(Mr.Prayoon Topart)

Authorized Signatory



ID LINE : IEC17025



Calibration Report

Certificate Number : SPR24030065-3

Page : 2 of 3

Reference Standards

Equipment Name	Model	Serial No.	Certificate No.	Due. Date
Sound Level Calibrator	ST-120	211203773	EEL.BP. 140/0167	26 Jan 2025

Traceability

This certification is traceable to the International System of Unit maintained at :

TISTR - Thailand Institute of Scientific and Technological Research



ID LINE : IEC17025



Result of Calibration

Certificate No. : SPR24030065-3

Page : 3 of 3

Range : 94 to 114 dB

Function : @1kHz

Select A

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.2	94.2	0.2	0.2	0.15
114	114.0	114.0	0.0	0.0	0.15

Select C

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.2	94.2	0.2	0.2	0.15
114	114.0	114.0	0.0	0.0	0.15

Note:

The result of calibration was found accurate as show on date and place of calibration only.
This Certificate is not certified for any commercial transaction.

Measurement Uncertainty

The reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor $k = 2.00$, providing a level of confidence approximately 95%.

- End of Certificate -



Certificate of Calibration

Certificate Number : SPR23120008-1

Page : 1 of 3

Customer : ENVIRPRO CO.,LTD.

168/28 Nakniwas Road., Ladprao, Ladprao, Bangkok 10230

Equipment Name : Noise Dose Meter

Manufacturer : Tenmars

Model : ST-130

Serial Number : 220100038

ID. Number : N/A

Environmental Conditions

Ambient Temperature : $23^{\circ}\text{C} \pm 3^{\circ}\text{C}$

Received Date : 01 Dec 2023

Relative Humidity : $50\% \pm 15\%$

Calibration Date : 04 Dec 2023

Location of Calibration : In-Lab

Recommend Due Date : N/A

Calibration Procedure : SP-CPE-04-01

Date of Issue : 05 Dec 2023

Method of Calibration


This certifies that the above instrument was calibrated in compliance with the calibration system requirement of ISO/IEC 17025:2017 in accordance with reference procedure. Standards used to perform this calibration are certified by to NIST or equivalent, National metrology institute, Natural physical constants, consensus standards. The result reported herein apply only to the calibration of the item described above as received. Our decision rule is to contact the customer if the item pass and fail calibration when the results include the uncertainties and the customer must determine if the results meets their needs.

The calibration certificate shall not be reproduced except in full, without written approval of SP Metrology System (Thailand).

Calibrated by : Mr.Karoon Pengsalung

Calibration Officer

Approved by :


(Mr.Prayoon Topart)

Authorized Signatory



Calibration Report

Certificate Number : SPR23120008-1

Page : 2 of 3

Reference Standards

Equipment Name	Model	Serial No.	Certificate No.	Due. Date
Sound Level Calibrator	ST-120	211203773	EEL.BP. 114/0166	17 Jan 2024

Traceability

This certification is traceable to the International System of Unit maintained at :
TISTR - Thailand Institute of Scientific and Technological Research

Envirpro



Result of Calibration

Certificate No. : SPR23120008-1

Range : 94 to 114 dB

Select ☒ A

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.0	94.0	0.0	0.0	0.15
114	113.7	113.7	-0.3	-0.3	0.15

Select C

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.0	94.0	0.0	0.0	0.15
114	114.0	114.0	0.0	0.0	0.15

Select Z

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.0	94.0	0.0	0.0	0.15
114	114.0	114.0	0.0	0.0	0.15

Note:

The result of calibration was found accurate as show on date and place of calibration only.
This Certificate is not certified for any commercial transaction.

Measurement Uncertainty

The reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor $k = 2.00$, providing a level of confidence approximately 95%.

– End of Certificate –



Certificate of Calibration

Certificate Number : SPR23120008-2

Page : 1 of 3

Customer : ENVIRPRO CO.,LTD.

168/28 Nakniwas Road., Ladprao, Ladprao, Bangkok 10230

Equipment Name : Noise Dose Meter

Manufacturer : Tenmars

Model : ST-130

Serial Number : 220100039

ID. Number : N/A

Environmental Conditions

Ambient Temperature : 23 °C \pm 3 °C

Received Date : 01 Dec 2023

Relative Humidity : 50 % \pm 15 %

Calibration Date : 04 Dec 2023

Location of Calibration : In-Lab

Recommend Due Date : N/A

Calibration Procedure : SP-CPE-04-01

Date of Issue : 05 Dec 2023

Method of Calibration

This certifies that the above instrument was calibrated in compliance with the calibration system requirement of ISO/IEC 17025:2017 in accordance with reference procedure. Standards used to perform this calibration are certified by to NIST or equivalent, National metrology institute, Natural physical constants, consensus standards. The result reported herein apply only to the calibration of the item described above as received. Our decision rule is to contact the customer if the item pass and fail calibration when the results include the uncertainties and the customer must determine if the results meets their needs.

The calibration certificate shall not be reproduced except in full, without written approval of SP Metrology System (Thailand).

Calibrated by : Mr.Karoon Pengsalung

Calibration Officer

Approved by :

(Mr.Prayoon Topart)

Authorized Signatory



Calibration Report

Certificate Number : SPR23120008-2

Page : 2 of 3

Reference Standards

Equipment Name	Model	Serial No.	Certificate No.	Due. Date
Sound Level Calibrator	ST-120	211203773	EEL.BP. 114/0166	17 Jan 2024

Traceability

This certification is traceable to the International System of Unit maintained at :
TISTR - Thailand Institute of Scientific and Technological Research

Envirpro



Result of Calibration

Certificate No. : SPR23120008-2

Page : 3 of 3

Range : 94 to 114 dB

Function : @1kHz

Select A

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.0	94.0	0.0	0.0	0.15
114	114.0	114.0	0.0	0.0	0.15

Select C

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.0	94.0	0.0	0.0	0.15
114	114.0	114.0	0.0	0.0	0.15

Select Z

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.0	94.0	0.0	0.0	0.15
114	114.0	114.0	0.0	0.0	0.15

Note:

The result of calibration was found accurate as show on date and place of calibration only.
This Certificate is not certified for any commercial transaction.

Measurement Uncertainty

The reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor $k = 2.00$, providing a level of confidence approximately 95%.

– End of Certificate –



Certificate Number : SPR23120008-3

Customer : ENVIRPRO CO.,LTD.

Page : 1 of 3

168/28 Nakniwas Road., Ladprao, Ladprao, Bangkok 10230

Equipment Name	: Noise Dose Meter
Manufacturer	: Tenmars
Model	: ST-130
Serial Number	: 220100040
ID. Number	: N/A

Environmental Conditions

Ambient Temperature : $23\text{ }^{\circ}\text{C} \pm 3\text{ }^{\circ}\text{C}$

Received Date : 01 Dec 2023

Relative Humidity : 50 % \pm 15 %

Calibration Date : 04 Dec 2023

Location of Calibration : In-Lab

Recommend Due Date : N/A

Calibration Procedure : SP-CPE-04-01

Date of Issue : 05 Dec 2023

Method of Calibration

This certifies that the above instrument was calibrated in compliance with the calibration system requirement of ISO/IEC 17025:2017 in accordance with reference procedure. Standards used to perform this calibration are certified by to NIST or equivalent, National metrology institute, Natural physical constants, consensus standards. The result reported herein apply only to the calibration of the item described above as received. Our decision rule is to contact the customer if the item pass and fail calibration when the results include the uncertainties and the customer must determine if the results meets their needs.

The calibration certificate shall not be reproduced except in full, without written approval of SP Metrology System (Thailand).

Calibrated by : Mr.Karoon Pengsalung

Calibration Officer

Approved by :

(Mr.Prayoon Topart)

Authorized Signatory



Calibration Report

Certificate Number : SPR23120008-3

Page : 2 of 3

Reference Standards

Equipment Name	Model	Serial No.	Certificate No.	Due. Date
Sound Level Calibrator	ST-120	211203773	EEL.BP. 114/0166	17 Jan 2024

Traceability

This certification is traceable to the International System of Unit maintained at :
TISTR - Thailand Institute of Scientific and Technological Research

Envirpro Co., Ltd.



Result of Calibration

Certificate No. : SPR23120008-3

Page : 3 of 3

Range : 94 to 114 dB

Function : @1kHz

Select A

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.0	94.0	0.0	0.0	0.15
114	113.8	113.8	-0.2	-0.2	0.15

Select C

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.0	94.0	0.0	0.0	0.15
114	113.9	113.9	-0.1	-0.1	0.15

Select Z

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.0	94.0	0.0	0.0	0.15
114	113.9	113.9	-0.1	-0.1	0.15

Note:

The result of calibration was found accurate as show on date and place of calibration only.
This Certificate is not certified for any commercial transaction.

Measurement Uncertainty

The reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor $k = 2.00$, providing a level of confidence approximately 95%.

- End of Certificate -



Certificate of Calibration

Certificate Number : SPR23120008-4

Page : 1 of 3

Customer : ENVIRPRO CO.,LTD.

168/28 Nakniwas Road., Ladprao, Ladprao, Bangkok 10230

Equipment Name : Noise Dose Meter

Manufacturer : Tenmars

Model : ST-130

Serial Number : 220100041

ID. Number : N/A

Environmental Conditions

Ambient Temperature : $23^{\circ}\text{C} \pm 3^{\circ}\text{C}$

Received Date : 01 Dec 2023

Relative Humidity : $50\% \pm 15\%$

Calibration Date : 04 Dec 2023

Location of Calibration : In-Lab

Recommend Due Date : N/A

Calibration Procedure : SP-CPE-04-01

Date of Issue : 05 Dec 2023

Method of Calibration

This certifies that the above instrument was calibrated in compliance with the calibration system requirement of ISO/IEC 17025:2017 in accordance with reference procedure. Standards used to perform this calibration are certified by to NIST or equivalent, National metrology institute, Natural physical constants, consensus standards. The result reported herein apply only to the calibration of the item described above as received. Our decision rule is to contact the customer if the item pass and fail calibration when the results include the uncertainties and the customer must determine if the results meets their needs.

The calibration certificate shall not be reproduced except in full, without written approval of SP Metrology System (Thailand).

Calibrated by : Mr.Karoon Pengsalung

Calibration Officer

Approved by :

(Mr.Prayoon Topart)

Authorized Signatory



Calibration Report

Certificate Number : SPR23120008-4

Page : 2 of 3

Reference Standards

Equipment Name	Model	Serial No.	Certificate No.	Due. Date
Sound Level Calibrator	ST-120	211203773	EEL.BP. 114/0166	17 Jan 2024

Traceability

This certification is traceable to the International System of Unit maintained at :
TISTR - Thailand Institute of Scientific and Technological Research

Envirpro Co., Ltd.



Result of Calibration

Certificate No. : SPR23120008-4

Page : 3 of 3

Range : 94 to 114 dB

Function : @1kHz

Select A

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.0	94.0	0.0	0.0	0.15
114	113.8	113.8	-0.2	-0.2	0.15

Select C

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.0	94.0	0.0	0.0	0.15
114	113.8	113.8	-0.2	-0.2	0.15

Select Z

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.0	94.0	0.0	0.0	0.15
114	113.8	113.8	-0.2	-0.2	0.15

Note:

The result of calibration was found accurate as show on date and place of calibration only.
This Certificate is not certified for any commercial transaction.

Measurement Uncertainty

The reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor $k = 2.00$, providing a level of confidence approximately 95%.

- End of Certificate -



Certificate of Calibration

Certificate Number : SPR23120008-5

Page : 1 of 3

Customer : ENVIRPRO CO.,LTD.

168/28 Nakniwas Road., Ladprao, Ladprao, Bangkok 10230

Equipment Name : Noise Dose Meter

Manufacturer : Tenmars

Model : ST-130

Serial Number : 220100042

ID. Number : N/A

Environmental Conditions

Ambient Temperature : $23^{\circ}\text{C} \pm 3^{\circ}\text{C}$

Received Date : 01 Dec 2023

Relative Humidity : $50\% \pm 15\%$

Calibration Date : 04 Dec 2023

Location of Calibration : In-Lab

Recommend Due Date : N/A

Calibration Procedure : SP-CPE-04-01

Date of Issue : 05 Dec 2023

Method of Calibration


This certifies that the above instrument was calibrated in compliance with the calibration system requirement of ISO/IEC 17025:2017 in accordance with reference procedure. Standards used to perform this calibration are certified by to NIST or equivalent, National metrology institute, Natural physical constants, consensus standards. The result reported herein apply only to the calibration of the item described above as received. Our decision rule is to contact the customer if the item pass and fail calibration when the results include the uncertainties and the customer must determine if the results meets their needs.

The calibration certificate shall not be reproduced except in full, without written approval of SP Metrology System (Thailand).

Calibrated by : Mr.Karoon Pengsalung

Calibration Officer

Approved by :


(Mr.Prayoon Topart)

Authorized Signatory



Calibration Report

Certificate Number : SPR23120008-5

Page : 2 of 3

Reference Standards

Equipment Name	Model	Serial No.	Certificate No.	Due. Date
Sound Level Calibrator	ST-120	211203773	EEL.BP. 114/0166	17 Jan 2024

Traceability

This certification is traceable to the International System of Unit maintained at :
TISTR - Thailand Institute of Scientific and Technological Research

Envirpro Co., Ltd.



Result of Calibration

Certificate No. : SPR23120008-5

Page : 3 of 3

Range : 94 to 114 dB

Function : @1kHz

Select A

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.0	94.0	0.0	0.0	0.15
114	113.8	113.8	-0.2	-0.2	0.15

Select C

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.0	94.0	0.0	0.0	0.15
114	113.8	113.8	-0.2	-0.2	0.15

Select Z

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.0	94.0	0.0	0.0	0.15
114	113.8	113.8	-0.2	-0.2	0.15

Note:

The result of calibration was found accurate as show on date and place of calibration only.
This Certificate is not certified for any commercial transaction.

Measurement Uncertainty

The reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor $k = 2.00$, providing a level of confidence approximately 95%.

- End of Certificate -



Certificate of Calibration

Certificate Number : SPR23120008-6

Page : 1 of 3

Customer : ENVIRPRO CO.,LTD.

168/28 Nakniwas Road., Ladprao, Ladprao, Bangkok 10230

Equipment Name : Noise Dose Meter

Manufacturer : Tenmars

Model : ST-130

Serial Number : 220100043

ID. Number : N/A

Environmental Conditions

Ambient Temperature : $23^{\circ}\text{C} \pm 3^{\circ}\text{C}$

Received Date : 01 Dec 2023

Relative Humidity : $50\% \pm 15\%$

Calibration Date : 04 Dec 2023

Location of Calibration : In-Lab

Recommend Due Date : N/A

Calibration Procedure : SP-CPE-04-01

Date of Issue : 05 Dec 2023

Method of Calibration

This certifies that the above instrument was calibrated in compliance with the calibration system requirement of ISO/IEC 17025:2017 in accordance with reference procedure. Standards used to perform this calibration are certified by to NIST or equivalent, National metrology institute, Natural physical constants, consensus standards. The result reported herein apply only to the calibration of the item described above as received. Our decision rule is to contact the customer if the item pass and fail calibration when the results include the uncertainties and the customer must determine if the results meets their needs.

The calibration certificate shall not be reproduced except in full, without written approval of SP Metrology System (Thailand).

Calibrated by : Mr.Karoon Pengsalung

Calibration Officer

Approved by :

(Mr.Prayoon Topart)

Authorized Signatory



Calibration Report

Certificate Number : SPR23120008-6

Page : 2 of 3

Reference Standards

Equipment Name	Model	Serial No.	Certificate No.	Due. Date
Sound Level Calibrator	ST-120	211203773	EEL.BP. 114/0166	17 Jan 2024

Traceability

This certification is traceable to the International System of Unit maintained at :
TISTR - Thailand Institute of Scientific and Technological Research

Enviropro



Result of Calibration

Certificate No. : SPR23120008-6

Page : 3 of 3

Range : 94 to 114 dB

Function : @1kHz

Select A

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.0	94.0	0.0	0.0	0.15
114	114.0	114.0	0.0	0.0	0.15

Select C

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.0	94.0	0.0	0.0	0.15
114	114.0	114.0	0.0	0.0	0.15

Select Z

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.0	94.0	0.0	0.0	0.15
114	114.0	114.0	0.0	0.0	0.15

Note:

The result of calibration was found accurate as show on date and place of calibration only.
This Certificate is not certified for any commercial transaction.

Measurement Uncertainty

The reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor $k = 2.00$, providing a level of confidence approximately 95%.

- End of Certificate -



Certificate of Calibration

Certificate Number : SPR23120008-7

Page : 1 of 3

Customer : ENVIRPRO CO.,LTD.

168/28 Nakniwas Road., Ladprao, Ladprao, Bangkok 10230

Equipment Name : Noise Dose Meter

Manufacturer : Tenmars

Model : ST-130

Serial Number : 220100044

ID. Number : N/A

Environmental Conditions

Ambient Temperature : $23^{\circ}\text{C} \pm 3^{\circ}\text{C}$

Received Date : 01 Dec 2023

Relative Humidity : $50\% \pm 15\%$

Calibration Date : 04 Dec 2023

Location of Calibration : In-Lab

Recommend Due Date : N/A

Calibration Procedure : SP-CPE-04-01

Date of Issue : 05 Dec 2023

Method of Calibration


This certifies that the above instrument was calibrated in compliance with the calibration system requirement of ISO/IEC 17025:2017 in accordance with reference procedure. Standards used to perform this calibration are certified by to NIST or equivalent, National metrology institute, Natural physical constants, consensus standards. The result reported herein apply only to the calibration of the item described above as received. Our decision rule is to contact the customer if the item pass and fail calibration when the results include the uncertainties and the customer must determine if the results meets their needs.

The calibration certificate shall not be reproduced except in full, without written approval of SP Metrology System (Thailand).

Calibrated by : Mr.Karoon Pengsalung

Calibration Officer

Approved by :


(Mr.Prayoon Topart)

Authorized Signatory



Calibration Report

Certificate Number : SPR23120008-7

Page : 2 of 3

Reference Standards

Equipment Name	Model	Serial No.	Certificate No.	Due. Date
Sound Level Calibrator	ST-120	211203773	EEL.BP. 114/0166	17 Jan 2024

Traceability

This certification is traceable to the International System of Unit maintained at :
TISTR - Thailand Institute of Scientific and Technological Research

Enviropro



Result of Calibration

Certificate No. : SPR23120008-7

Page : 3 of 3

Range : 94 to 114 dB

Function : @1kHz

Select A

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.0	94.0	0.0	0.0	0.15
114	113.8	113.8	-0.2	-0.2	0.15

Select C

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.0	94.0	0.0	0.0	0.15
114	113.8	113.8	-0.2	-0.2	0.15

Select Z

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.0	94.0	0.0	0.0	0.15
114	113.9	113.9	-0.1	-0.1	0.15

Note:

The result of calibration was found accurate as show on date and place of calibration only.
This Certificate is not certified for any commercial transaction.

Measurement Uncertainty

The reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor $k = 2.00$, providing a level of confidence approximately 95%.

- End of Certificate -



Certificate of Calibration

Certificate Number : SPR23120008-8

Page : 1 of 3

Customer : ENVIRPRO CO.,LTD.

168/28 Nakniwas Road., Ladprao, Ladprao, Bangkok 10230

Equipment Name : Noise Dose Meter

Manufacturer : Tenmars

Model : ST-130

Serial Number : 220100045

ID. Number : N/A

Environmental Conditions

Ambient Temperature : 23 °C \pm 3 °C

Received Date : 01 Dec 2023

Relative Humidity : 50 % \pm 15 %

Calibration Date : 04 Dec 2023

Location of Calibration : In-Lab

Recommend Due Date : N/A

Calibration Procedure : SP-CPE-04-01

Date of Issue : 05 Dec 2023

Method of Calibration


This certifies that the above instrument was calibrated in compliance with the calibration system requirement of ISO/IEC 17025:2017 in accordance with reference procedure. Standards used to perform this calibration are certified by to NIST or equivalent, National metrology institute, Natural physical constants, consensus standards. The result reported herein apply only to the calibration of the item described above as received. Our decision rule is to contact the customer if the item pass and fail calibration when the results include the uncertainties and the customer must determine if the results meets their needs.

The calibration certificate shall not be reproduced except in full, without written approval of SP Metrology System (Thailand).

Calibrated by : Mr.Karoon Pengsalung

Calibration Officer

Approved by :


(Mr.Prayoon Topart)

Authorized Signatory



Calibration Report

Certificate Number : SPR23120008-8

Page : 2 of 3

Reference Standards

Equipment Name	Model	Serial No.	Certificate No.	Due. Date
Sound Level Calibrator	ST-120	211203773	EEL.BP. 114/0166	17 Jan 2024

Traceability

This certification is traceable to the International System of Unit maintained at :
TISTR - Thailand Institute of Scientific and Technological Research

Envirpro Co., Ltd.



Result of Calibration

Certificate No. : SPR23120008-8

Page : 3 of 3

Range : 94 to 114 dB

Function : @1kHz

Select A

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.0	94.0	0.0	0.0	0.15
114	113.8	113.8	-0.2	-0.2	0.15

Select C

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.0	94.0	0.0	0.0	0.15
114	113.9	113.9	-0.1	-0.1	0.15

Select Z

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.0	94.0	0.0	0.0	0.15
114	113.9	113.9	-0.1	-0.1	0.15

Note:

The result of calibration was found accurate as show on date and place of calibration only.
This Certificate is not certified for any commercial transaction.

Measurement Uncertainty

The reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor $k = 2.00$, providing a level of confidence approximately 95%.

- End of Certificate -



Certificate of Calibration

Page : 1 of 3

168/28 Nakniwas Road., Ladprao, Ladprao, Bangkok 10230

ID. Number : N/A

Date of Issue : 05 Dec 2023

The calibration certificate shall not be reproduced except in full, without written approval of SP Metrology System (Thailand).

(Mr.Prayoon Topart)

Authorized Signatory



Calibration Report

Certificate Number : SPR23120008-9

Page : 2 of 3

Reference Standards

Equipment Name	Model	Serial No.	Certificate No.	Due. Date
Sound Level Calibrator	ST-120	211203773	EEL.BP. 114/0166	17 Jan 2024

Traceability

This certification is traceable to the International System of Unit maintained at :
TISTR - Thailand Institute of Scientific and Technological Research

Enviropro



Result of Calibration

Certificate No. : SPR23120008-9

Page : 3 of 3

Range : 94 to 114 dB

Function : @1kHz

Select A

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.0	94.0	0.0	0.0	0.15
114	113.9	113.9	-0.1	-0.1	0.15

Select C

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.0	94.0	0.0	0.0	0.15
114	113.9	113.9	-0.1	-0.1	0.15

Select Z

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.0	94.0	0.0	0.0	0.15
114	114.0	114.0	0.0	0.0	0.15

Note:

The result of calibration was found accurate as show on date and place of calibration only.
This Certificate is not certified for any commercial transaction.

Measurement Uncertainty

The reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor $k = 2.00$, providing a level of confidence approximately 95%.

- End of Certificate -



Certificate of Calibration

Certificate Number : SPR23120008-10

Page : 1 of 3

Customer : ENVIRPRO CO.,LTD.

168/28 Nakniwas Road., Ladprao, Ladprao, Bangkok 10230

Equipment Name : Noise Dose Meter

Manufacturer : Tenmars

Model : ST-130

Serial Number : 220100047

ID. Number : N/A

Environmental Conditions

Ambient Temperature : 23 °C \pm 3 °C

Received Date : 01 Dec 2023

Relative Humidity : 50 % \pm 15 %

Calibration Date : 04 Dec 2023

Location of Calibration : In-Lab

Recommend Due Date : N/A

Calibration Procedure : SP-CPE-04-01

Date of Issue : 05 Dec 2023

Method of Calibration


This certifies that the above instrument was calibrated in compliance with the calibration system requirement of ISO/IEC 17025:2017 in accordance with reference procedure. Standards used to perform this calibration are certified by to NIST or equivalent, National metrology institute, Natural physical constants, consensus standards. The result reported herein apply only to the calibration of the item described above as received. Our decision rule is to contact the customer if the item pass and fail calibration when the results include the uncertainties and the customer must determine if the results meets their needs.

The calibration certificate shall not be reproduced except in full, without written approval of SP Metrology System (Thailand).

Calibrated by : Mr.Karoon Pengsalung

Calibration Officer

Approved by :


(Mr.Prayoon Topart)

Authorized Signatory



Calibration Report

Certificate Number : SPR23120008-10

Page : 2 of 3


Reference Standards

Equipment Name	Model	Serial No.	Certificate No.	Due. Date
Sound Level Calibrator	ST-120	211203773	EEL.BP. 114/0166	17 Jan 2024

Traceability

This certification is traceable to the International System of Unit maintained at :

TISTR - Thailand Institute of Scientific and Technological Research



Result of Calibration

Certificate No. : SPR23120008-10

Page : 3 of 3

Range : 94 to 114 dB

Function : @1kHz

Select A

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.0	94.0	0.0	0.0	0.15
114	113.8	113.8	-0.2	-0.2	0.15

Select C

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.0	94.0	0.0	0.0	0.15
114	113.8	113.8	-0.2	-0.2	0.15

Select Z

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.0	94.0	0.0	0.0	0.15
114	113.9	113.9	-0.1	-0.1	0.15

Note:

The result of calibration was found accurate as show on date and place of calibration only.
This Certificate is not certified for any commercial transaction.

Measurement Uncertainty

The reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor $k = 2.00$, providing a level of confidence approximately 95%.

– End of Certificate –

ภาคผนวก จ

สำเนาเอกสารกฎหมายที่เกี่ยวข้อง