

ภาคผนวก จ  
เอกสารสอบเทียบเครื่องมือวัด

---

### List of Instruments Certification for Air & Noise Quality Analysis

No.	Instrument/Equipment	Parameter	Manufacturer	Model/Serial No.	Calibrator	Certification No.	Date of Calibration	Due date of Calibration	Remark
<b>Ambient</b>									
1	Orifice Transfer Standard Calibrator	Total Suspended Particulate (TSP) Particulate Matter < 10 µm (PM <sub>10</sub> )	Andersen Instruments, Inc.	G25A 1901	Jiranatee Associates Co., Ltd.	COF-002-66	14 Jul 23	13 Jul 25	-
2	U-Tube Manometer	Total Suspended Particulate (TSP) Particulate Matter < 10 µm (PM <sub>10</sub> )	Dwyer	1221-36-W/M -	Technology Promotion Association (Thailand-Japan)	24P1251	11 Apr 24	10 Apr 25	-
3	Aneroid Barometer	Total Suspended Particulate (TSP) Particulate Matter < 10 µm (PM <sub>10</sub> )	Barigo, Germany	-	Technology Promotion Association (Thailand-Japan)	24P1369	22 Apr 24	21 Apr 25	-
4	Dial Thermo-Hygrometer	Total Suspended Particulate (TSP) Particulate Matter < 10 µm (PM <sub>10</sub> )	Barigo, Germany	-	Technology Promotion Association (Thailand-Japan)	24H753	10 Apr 24	9 Apr 25	-
5	Nitrogen Dioxide Analyzer	Nitrogen Dioxide	Thermo Environmental Instrument	42C 42C-78933-390	UAE Consultant Co.,Ltd.	20092024	20 Sep 24	19 Sep 25	-
6	Nitrogen Dioxide Analyzer	Nitrogen Dioxide	Thermo Environmental Instrument	42C 42C-58929-320	UAE Consultant Co.,Ltd.	04102024	4 Oct 24	3 Oct 25	-
7	Nitrogen Dioxide Analyzer	Nitrogen Dioxide	Thermo Scientific	42i 1180540062	UAE Consultant Co.,Ltd.	17102024	17 Oct 24	16 Oct 25	-
8	Nitrogen Dioxide Analyzer	Nitrogen Dioxide	Thermo Scientific	42i 1180540063	UAE Consultant Co.,Ltd.	17092024	17 Sep 24	16 Sep 25	-
9	Standard Gases (Mixture)	Nitrogen Dioxide	Airgas	EB0162121 2016PSIG	Airgas an Air Liquide company	E05NI91E15A0014	6 Jun 23	6 Jun 31	-
10	Sulphur Dioxide Analyzer	Sulphur Dioxide	Thermo Scientific	42i 1182920016	UAE Consultant Co.,Ltd.	06092024	6 Sep 24	5 Sep 25	-
11	Sulphur Dioxide Analyzer	Sulphur Dioxide	Thermo Scientific	43i 1182920017	UAE Consultant Co.,Ltd.	15062024	15 May 24	14 May 25	-
12	Sulphur Dioxide Analyzer	Sulphur Dioxide	Thermo Scientific	43i 1182920017	UAE Consultant Co.,Ltd.	09042024	4 Sep 24	3 Sep 25	-
13	Sulphur Dioxide Analyzer	Sulphur Dioxide	Thermo Scientific	43i 1180540065	UAE Consultant Co.,Ltd.	04092024	4 Sep 24	3 Sep 25	-

### List of Instruments Certification for Air & Noise Quality Analysis

No.	Instrument/Equipment	Parameter	Manufacturer	Model/Serial No.	Calibrator	Certification No.	Date of Calibration	Due date of Calibration	Remark
<b>Ambient</b>									
14	Standard Gases (Mixture)	Sulphur Dioxide	Airgas	EB0162121 2016PSIG	Airgas an Air Liquide company	E05NI91E15A0014	6 Jun 23	6 Jun 31	-
15	Carbon Monoxide Analyzer	Carbon Monoxide	Thermo	48i 1180540074	UAE Consultant Co.,Ltd.	09092024	9 Sep 24	8 Sep 25	-
16	Carbon Monoxide Analyzer	Carbon Monoxide	Horiba	APMA-370 YN43AG7T	UAE Consultant Co.,Ltd.	14062024	14 Jun 24	13 Jun 25	-
17	Carbon Monoxide Analyzer	Carbon Monoxide	Thermo	48i CM08140004	UAE Consultant Co.,Ltd.	03092024	3 Sep 24	2 Sep 25	-
18	Carbon Monoxide Analyzer	Carbon Monoxide	Thermo	48i 1182920018	UAE Consultant Co.,Ltd.	14062024	14 Jun 24	13 Jun 25	-
19	Standard Gases (Mixture)	Carbon Monoxide	Airgas	EB0162121 2016PSIG	Airgas an Air Liquide company	E05NI91E15A0014	6 Jun 23	6 Jun 31	-
20	Vibration Meter	Vibration Level Acceleration Level	Instantel Inc.	Micromate UM11056	Calibration Laboratory Co.Ltd	Q24037351	8 Apr 24	7 Apr 25	-
21	Vibration Meter	Vibration Level Acceleration Level	Instantel Inc.	Micromate UM11057	Calibration Laboratory Co.Ltd	Q24042939	30 Apr 24	29 Apr 25	-
22	Vibration Meter	Vibration Level Acceleration Level	Instantel Inc.	Micromate UM11058	Calibration Laboratory Co.Ltd	Q24037354	8 Apr 24	7 Apr 25	-
23	Vibration Meter	Vibration Level Acceleration Level	Instantel Inc.	Micromate UM11059	Calibration Laboratory Co.Ltd	Q24037352	8 Apr 24	7 Apr 25	-
24	Sound Level Calibrator (Acoustic Calibrator)	Calibrate Sound Level Meter	Svantek	SV36 107224	Innovative Instrument Co.,Ltd.	24-ACT-091	26 Jun 24	25 Jun 25	-
25	Sound Level Meter	$L_{Aeq\ 1\ hours}$ , $L_{Aeq\ 24\ hrs}$ , $L_{Amax}$ , $L_{A90}$	Larson Davis	LxT2 0005286	Innovative Instrument Co.,Ltd.	24-SLM-234	10 Jul 24	9 Jul 25	-
26	Sound Level Meter	$L_{Aeq\ 1\ hours}$ , $L_{Aeq\ 24\ hrs}$ , $L_{Amax}$ , $L_{A90}$	Larson Davis	LxT2 0005290	Innovative Instrument Co.,Ltd.	24-SLM-238	11 Jul 24	10 Jul 25	-

List of Instruments Certification for Air & Noise Quality Analysis

No.	Instrument/Equipment	Parameter	Manufacturer	Model/Serial No.	Calibrator	Certification No.	Date of Calibration	Due date of Calibration	Remark
Ambient									
27	Sound Level Meter	L <sub>Aeq</sub> 1 hours, L <sub>Aeq</sub> 24 hrs, L <sub>Amax</sub> , L <sub>A90</sub>	Larson Davis	LxT2	Innovative Instrument Co.,Ltd.	24-SLM-231	10 Jul 24	9 Jul 25	-
				0005293					
28	Sound Level Meter	L <sub>Aeq</sub> 1 hours, L <sub>Aeq</sub> 24 hrs, L <sub>Amax</sub> , L <sub>A90</sub>	Larson Davis	LxT2	Innovative Instrument Co.,Ltd.	24-SLM-240	11 Jul 24	10 Jul 25	-
				0005299					



## CERTIFICATE OF CALIBRATION

Certificate No. : COF-002-66

Page 1 of 2 Pages

**MEASUREMENT ITEM** : Top Load Orifice  
**MANUFACTURER** : Andersen Instruments  
**MODEL/TYPE** : G25A  
**SERIAL NUMBER** : 1901  
**ID NUMBER** : UAE.ANV.051/2547  
**CONDITION AS-RECEIVED** : Used item  
**CUSTOMER** : United Analyst and Engineering Consultant Co., Ltd.  
81 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong,  
Bangkok 10260

**Calibration procedure:**  
The Orifice gas flow device was calibrated against  
Standard Rotary Displacement Meter (Roots  
Meter) Model G65/IMC/W2-dp. The W1-G1-004  
was used as a calibration guideline.

**Traceability:**  
This certificate provides a traceability of The  
measurement to recognized the national  
standards, and to realization of the international  
system of units (SI) through the VSL (National  
Metrology Institute of Netherlands) via Certificate  
number: G2211901

**Uncertainty of Measurement:**  
The reported uncertainty of measurement is based  
on the standard uncertainty multiplied by a  
coverage factor  $k=2$ . Which for a normal  
distribution corresponds to a coverage probability  
of approximately 95%. The standard uncertainty  
has been determined in accordance with the GUM  
Evaluation of measurement  
data - Guide to the expression of uncertainty in  
measurement

**RECEIVED DATE** : 07 Jul 2023  
**MEASUREMENT DATE** : 14 Jul 2023  
**ISSUE DATE** : 18 Jul 2023

**ENVIRONMENTAL CONDITIONS:**  
Ambient condition in the laboratory are as follow:  
Temperature :  $23.0 \pm 3.0$  °C  
Relative Humidity :  $55.0 \pm 15.0$  %RH  
Atmospheric Pressure :  $1010 \pm 10$  hPa

**CALIBRATION CONDITION:**  
Preconditioning : 24 hours at ambient conditions.  
Measurement Condition : The average values during measurement are 23.9 °C and 54.5%RH.


**NOTED:** The certificate is valid only to the item calibrated on date and place of calibration.

**TABULATION OF RESULTS:**  
The table on next page give the measured values.

Calibrated by:  
☐ Mr. Sorawit Thachalad  
☒ Miss Jitraporn Lertsomphol



Approved signatory:



เอกสารไม่ควบคุม

THIS CERTIFICATE REPORT MAY NOT BE REPRODUCED EXCEPT IN FULL UNLESS PERMISSION FOR REPRODUCTION HAS BEEN OBTAINED  
IN WRITING FROM THE LABORATORY

### MEASUREMENT RESULTS:

The Orifice gas flow device was calibrated by direct comparison method with the Standard Rotary Displacement Meter (Roots Meter). The Humid air was used as a medium in the system. The standard conditions are 25°C (298.15 K) and 760 mmHg for standard temperature and standard pressure respectively.

Table 1: The results of  $Q$  Standard calibration data

Plate	Flow rate $m^3/min$	Pressure [Pa] mmHg	Temperature [Ta] °C	Temperature [Tm] °C	$\Delta p_{meter}$ mmHg	$\Delta p_{Orifice}$ inH <sub>2</sub> O	$\gamma$	Standard Flow [ $Q_s$ ] $m^3/min$
1	0.701	754.115	23.87	23.10	55.600	1.626	1.273	0.648
2	0.997	754.083	23.80	23.23	61.350	3.236	1.795	0.914
3	1.121	754.005	23.81	23.20	41.923	4.338	2.079	1.057
4	1.172	754.004	23.72	23.16	30.933	4.891	2.208	1.122
5	1.410	753.994	23.76	23.18	29.415	7.159	2.671	1.352

Slope (m): 1.98463  
Intercept (k): -0.01636  
Correlation coefficient (r): 0.99972  
Uncertainty ( $k=2$ ): 0.015  $m^3/min$

Table 2: The results of  $Q$  actual calibration data

Plate	Flow rate $m^3/min$	Pressure [Pa] mmHg	Temperature [Ta] °C	Temperature [Tm] °C	$\Delta p_{meter}$ mmHg	$\Delta p_{Orifice}$ inH <sub>2</sub> O	$\gamma$	Standard Flow [ $Q_s$ ] $m^3/min$
1	0.701	754.115	23.87	23.10	55.600	1.626	0.800	0.651
2	0.997	754.083	23.80	23.23	61.350	3.236	1.129	0.917
3	1.121	754.005	23.81	23.20	41.923	4.338	1.307	1.061
4	1.172	754.004	23.72	23.16	30.933	4.891	1.388	1.126
5	1.410	753.994	23.76	23.18	29.415	7.159	1.679	1.357

Slope (m): 1.24306  
Intercept (k): -0.01029  
Correlation coefficient (r): 0.99972  
Uncertainty ( $k=2$ ): 0.015  $m^3/min$

\*\*\*End of Certificate of Calibration\*\*\*



เอกสารไม่ควบคุม



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)  
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES  
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG, BANGKOK 10250  
TEL. 0-2717-3000-24 FAX. 0-2719-9484

## Certificate of Calibration

Certificate No. : 24P1251  
Page : 1 of 2

**Equipment :** U Tube Manometer  
**Manufacturer:** Dwyer  
**Model :** 1221-36-W/M  
**Serial No.:** -  
**ID No.:** UAE.EFM.077/2566

**Condition As-Received:** Used Item  
**Received Date:** 03 April 2024  
**Calibration Date:** 11 April 2024

**Reference:** 2404-0118WSC  
**Ambient Temperature:** (  $23 \pm 2$  ) °C  
**Relative Humidity:** (  $50 \pm 15$  ) %  
**Atmospheric Pressure:** 1012 mbar

**Submitted by:** United Analyst and Engineering Consultant Co.,Ltd.  
81 Soi Udomsuk 41, Sukhumvit Road, Bangchak,  
Phrakhanong, Bangkok 10260

**Procedure used:** The calibration was conducted by direct comparison method against Pressure Measuring Instruments  
Standard according to calibration procedure CP-P04, using " DKD-R 6-1 ; Calibration of Pressure Gauges " as  
a guidelines.

### Condition of this result of calibration

1.Reference standards instruments :

Instrument	Model	Serial No.	Certificate No.	Due Date
1) Pressure Calibrator	PC106P	1189	MP-0176-23	12 Sep 2024

2.This result of calibration was made on requested at the point specified by customer.

3.Scale and conversion factor is 1 kPa = 4.0146293 inH<sub>2</sub>O

4.This instrument was used clean air as pressure media.

5.This instrument was calibrated by applied pressure to high-port (+) side and low-port (-) side open to atmospheric pressure.

6.This instrument was installed in vertical orientation and top of the pressure port was used as the reference level.

7.The certificate is valid only to the item calibrated on date and place of calibration.

8.This Certification is traceable to the International System of Unit maintained through-

-National Institute of Metrology (Thailand), NSC-ONSC Accredited No, Calibration 0144

**Calibrated by :** Suksan Khankaew  
**Issue Date :** 17 April 2024

**Approved Signatory :**  
[ ] Phalinee Prathpalap  
[ ] Sura Suwannasri  
[✓] Attapol Panurach

เอกสารไม่ควบคุม



Cert.No.: 24P1251  
Page: 2 of 2

**Result of calibration:- Without adjustment**  
**Function:- Pressure Measurement**  
**Increasing Pressure**

**Range :** 0 inH<sub>2</sub>O to 36 inH<sub>2</sub>O  
**Scale Interval :** 0.1 inH<sub>2</sub>O ( The Second Estimate )

Applied Pressure	High-port side	UUC Indication Low-port side	$\Delta P$	Error
0.00	0.00	0.00	0.00	0.00
2.00	1.00	-1.00	2.00	0.00
4.00	2.00	-2.00	4.00	0.00
6.00	3.00	-3.00	6.00	0.00
8.00	4.00	-4.00	8.00	0.00
10.00	5.00	-5.00	10.00	0.00
12.00	6.00	-6.00	12.00	0.00
14.00	7.05	-7.05	14.10	0.10
16.00	8.05	-8.05	16.10	0.10
18.00	9.05	-9.05	18.10	0.10
20.00	10.05	-10.05	20.10	0.10
22.00	11.05	-11.05	22.10	0.10
24.00	12.05	-12.05	24.10	0.10
26.00	13.05	-13.05	26.10	0.10
28.00	14.05	-14.05	28.10	0.10
30.00	15.05	-15.05	30.10	0.10
32.00	16.05	-16.10	32.15	0.15
34.00	17.05	-17.10	34.15	0.15
35.80	18.00	-18.00	36.00	0.20

The uncertainty of measurement was  $\pm 0.11$  inH<sub>2</sub>O

\*  $\Delta P$  = High-port side - Low-port side


\* UUC = Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied  
by a coverage factor  $k=2$ , providing a level of confidence of approximately 95 %.

-000-

เอกสารไม่ควบคุม





Certificate No. : 24P1369  
Page : 1 of 2

This certificate may not be reproduced other than in full, except with the prior written approval of the head of Corporate Services 3: Equipment Calibration and Testing Services.

<b>Reference:</b>	2404-0243WSC	<b>Submitted by:</b>	United Analyst and Engineering Consultant Co.,Ltd.
<b>Ambient Temperature:</b>	( 23 ± 2 ) °C		
<b>Relative Humidity:</b>	( 50 ± 15 ) %		81 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
<b>Atmospheric Pressure:</b>	1007 mbar		

**Procedure used:** The calibration was conducted by direct comparison method against Pressure Measuring Instruments Standard according to calibration procedure CP-P10, using "DKD-R 6-1 ; Calibration of Pressure Gauges" as a guidelines.

**Condition of this result of calibration**

1. Reference standards instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Certificate No.</u>	<u>Due Date</u>
meter	DPI142	1422505046	MP-0094-23	03 May 2024

2. This instrument was installed in vertical orientation and center of the dial was used as the reference level.

3. This result of calibration was made on requested at the point specified by customer.

4. Scale and conversion factor is  $1 \text{ kPa} = 7.50062 \text{ mmHg}$

5. This result of calibration instrument was in absolute pressure.

6. This instrument was used clean air as pressure media.

7. The certificate is valid only to the item calibrated on date and place of calibration.

8.This Certification is traceable to the International System of Unit maintained through:-

-National Institute of Metrology Thailand (NIMT)

Calibrated by : Suksan Khankaew  
Issue Date : 23 April 2024


Approved Signatory : \_\_\_\_\_

[ ] Phalinee Prabpaipal

[ ] Sura Suwannasri

[✓] Attapol Panurach

## เอกสารไม่ควบคุม



Certificate No. : 24H753  
Page : 1 of 2

This certificate may not be reproduced other than in full, except with the prior written approval of the head of Corporate Services 3: Equipment Calibration and Testing Services.

<b>Reference:</b>	W 16 April 2024 2404-0247WSC	<b>Submitted by:</b>	United Analyst and Engineering Consultant Co.,Ltd.
<b>Ambient Temperature:</b>	( 25 ± 3 ) °C		
<b>Relative Humidity:</b>	( 50 ± 20 ) %		81 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260

**Procedure used:** Calibration were conducted using in-house calibration procedure CP-H02 according to comparison with standard chilled mirror sensor for humidity measurement function and comparison with standard temperature probe for temperature measurement function into humidity / temperature chamber.

**Condition of this result of calibration**

1.Reference standards instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Certificate No.</u>	<u>Due Date</u>
grometer	Dew Master	44730	21656	02 Aug 2024
ometer With Sensor	1521	A5A339	231238	16 Oct 2024

2. The certificate is valid only to the item calibrated on date and place of calibration.

3.This Certification is traceable to the International System of Unit maintained through:-

-Thunder Scientific Corporation, NVLAB Accreditation No. Calibration 200582-0

-Technology Promotion Association (Thailand-Japan), NSC-ONSC Accredited No. Calibration 0008

**Calibrated by :** Chakrit Waewwanjua  
**Issue Date :** 18 April 2024

Approved Signatory : \_\_\_\_\_

☐ Chakrit Waewwanjua

☒ Viporn Tantiyawutti

☐ Unnopphol Harachai

## เอกสารไม่ควบคุม

**Result of Calibration:-** Without Adjustment  
**Function:** Humidity Measurement.

Reference Temperature	Standard Humidity	UUC* Reading	Error	Uncertainty of Measurement
(°C)	(%R.H.)	(%R.H.)	(%R.H.)	(±%R.H.)
25.0	40.1	43	2.9	1.6
25.0	60.0	60	0.0	1.7
25.0	80.0	78	-2.0	1.8

**Result of Calibration:-** Without Adjustment  
**Function:** Temperature Measurement.

Standard <u>Temperature</u>	UUC* <u>Reading</u>	<u>Error</u>	Uncertainty <u>of Measurement</u>
(°C)	(°C)	(°C)	(±°C)
20,014	20.0	-0.014	0.72
25,033	25.0	-0.033	0.72
30,010	30.0	-0.010	0.72
35,027	34.5	-0.527	0.72
40,013	39.5	-0.513	0.72

**UUC\*** : Unit Under Calibration

The reported uncertainty of measurement was base on standard uncertainty multiplied by coverage factor  $k = 2.00$ , providing confidence level approximately 95%.

-o0o-

## เอกสารไม่ควบคุม

### MULTI-POINT GAS TEST REPORT

Test Date : Sep 20, 2024

Equipment : Gas Analyzer (NO<sub>2</sub>) Model : 42C  
Manufacturer : Thermo Environmental Instruments Serial Number : 42C-78933-390

#### Standard Gas Concentration


Sulphur Dioxide (SO<sub>2</sub>) 42.89 PPM  
Nitric Oxide (NO) 46.77 PPM  
Methane (CH<sub>4</sub>) - PPM  
Carbon Monoxide (CO) 965.9 PPM  
Cylinder No. : EB0159156  
Expiration Date : Nov 6, 2026

#### Dilutor Detail

Manufacturer : Thermo Scientific  
Model : 146i  
Serial Number : 1180540071

#### Multi-point gas test data

	Reference Value (ppb)	Analyzer Display (ppb)	Difference Error	Percent Error	[% Error ]
Level 1	Zero	0.0	0.00	0.00	0.00
Level 2	20.00%	100.0	100.9	0.90	0.89
Level 3	40.00%	200.0	200.7	0.70	0.35
Level 4	60.00%	300.0	300.6	0.60	0.20
Level 5	80.00%	400.0	400.0	0.00	0.00
Remark : Measuring Range	500.0 ppb		Average Difference (%)		0.29
:Acceptable Limit $\pm 5\%$					

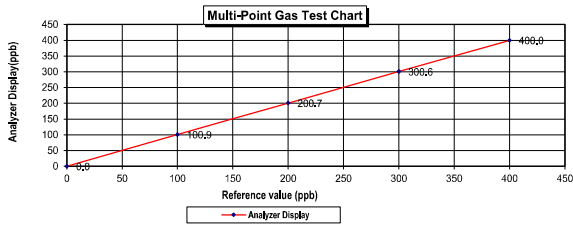

20 / 9 / 2567

20 / Sep / 2024

### MULTI-POINT GAS TEST REPORT

Test Date : Oct 4, 2024

Equipment : Gas Analyzer (NO<sub>2</sub>) Model : 42C  
Manufacturer : Thermo Environmental Instruments Serial Number : 42C-58929-320

#### Standard Gas Concentration


Sulphur Dioxide (SO<sub>2</sub>) 42.89 PPM  
Nitric Oxide (NO) 46.77 PPM  
Methane (CH<sub>4</sub>) - PPM  
Carbon Monoxide (CO) 965.9 PPM  
Cylinder No. : EB0159156  
Expiration Date : Nov 6, 2026

#### Dilutor Detail

Manufacturer : Thermo Scientific  
Model : 146i  
Serial Number : 1180540071

#### Multi-point gas test data

	Reference Value (ppb)	Analyzer Display (ppb)	Difference Error	Percent Error	[% Error ]
Level 1	Zero	0.0	0.00	0.00	0.00
Level 2	20.00%	100.0	100.5	0.50	0.50
Level 3	40.00%	200.0	200.8	0.80	0.40
Level 4	60.00%	300.0	300.7	0.70	0.23
Level 5	80.00%	400.0	400.0	0.00	0.00
Remark : Measuring Range	500.0 ppb		Average Difference (%)		0.23
:Acceptable Limit $\pm 5\%$					

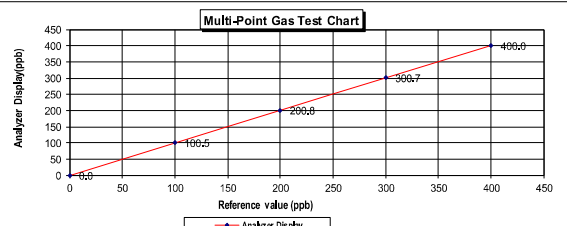

4 / 10 / 2567

4 / Oct / 2024

### MULTI-POINT GAS TEST REPORT

Test Date : Oct 17, 2024

Equipment : Gas Analyzer (NO<sub>2</sub>) Model : 42i  
Manufacturer : Thermo Scientific Serial Number : 1180540062

#### Standard Gas Concentration


Sulphur Dioxide (SO<sub>2</sub>) 42.89 PPM  
Nitric Oxide (NO) 46.77 PPM  
Methane (CH<sub>4</sub>) - PPM  
Carbon Monoxide (CO) 965.9 PPM  
Cylinder No. : EB0159156  
Expiration Date : Nov 6, 2026

#### Dilutor Detail

Manufacturer : Thermo Scientific  
Model : 146i  
Serial Number : 1180540071

#### Multi-point gas test data

	Reference Value (ppb)	Analyzer Display (ppb)	Difference Error	Percent Error	[% Error ]
Level 1	Zero	0.0	0.00	0.00	0.00
Level 2	20.00%	100.0	100.6	0.60	0.60
Level 3	40.00%	200.0	200.6	0.60	0.30
Level 4	60.00%	300.0	300.7	0.70	0.23
Level 5	80.00%	400.0	400.0	0.00	0.00
Remark : Measuring Range	500.0 ppb		Average Difference (%)		0.23
:Acceptable Limit $\pm 5\%$					

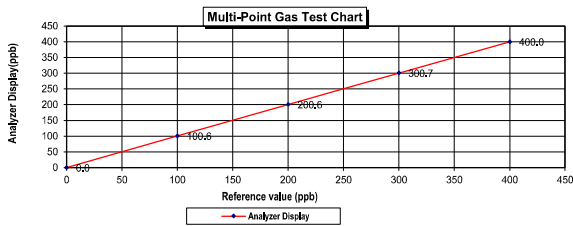

17 / 10 / 2567

17 / Oct / 2024

### MULTI-POINT GAS TEST REPORT

Test Date : Sep 17, 2024

Equipment : Gas Analyzer (NO<sub>2</sub>) Model : 42i  
Manufacturer : Thermo Scientific Serial Number : 1180540063

#### Standard Gas Concentration


Sulphur Dioxide (SO<sub>2</sub>) 42.89 PPM  
Nitric Oxide (NO) 46.77 PPM  
Methane (CH<sub>4</sub>) - PPM  
Carbon Monoxide (CO) 965.9 PPM  
Cylinder No. : EB0159156  
Expiration Date : Nov 06, 2026

#### Dilutor Detail

Manufacturer : Thermo Scientific  
Model : 146i  
Serial Number : 1180540071

#### Multi-point gas test data

	Reference Value (ppb)	Analyzer Display (ppb)	Difference Error	Percent Error	[% Error ]
Level 1	Zero	0.0	0.00	0.00	0.00
Level 2	20.00%	100.0	100.9	0.90	0.89
Level 3	40.00%	200.0	200.5	0.50	0.25
Level 4	60.00%	300.0	300.9	0.90	0.30
Level 5	80.00%	400.0	400.0	0.00	0.00
Remark : Measuring Range	500.0 ppb		Average Difference (%)		0.29
:Acceptable Limit $\pm 5\%$					

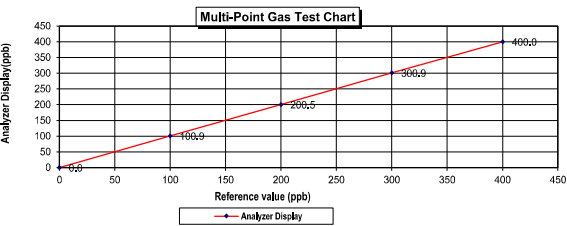

17 / 9 / 2567

17 / Sep / 2024



## CERTIFICATE OF ANALYSIS

## Grade of Product: EPA PROTOCOL STANDARD

Customer: AIR LIQUIDE (THAILAND)  
LTD--  
Part Number: E05NI91E15A0014  
Cylinder Number: EB0162121  
Laboratory: 124 - Plumsteadville - PA  
PGVP Number: A12023  
Gas Code: CO, CO2, NO, NOX, SO2, BALN

Reference Number: 160-40272205-1  
Cylinder Volume: 144.0 CF  
Cylinder Pressure: 2016 PSIG  
Valve Outlet: 660  
Certification Date: Jul 06, 2023

Expiration Date: Jul 06, 2031

Certification performed in accordance with "EPA Traceability Protocol" for Assay and Certification of Gaseous Calibration Standards (May 2012) document EPA 800/R-12/531, using the assay procedures listed. Analytical Methodology does not require correction for analytical interference. This cylinder has a total analytical uncertainty as stated below with a confidence level of 95%. There are no significant impurities which affect the use of this calibration mixture. All concentrations are on a mole/mole basis unless otherwise noted. The results relate only to the items tested. The report shall not be reproduced except in full without approval of the laboratory. Do Not Use This Cylinder below 100 psig, i.e. 0.7 megapascals.

ANALYTICAL RESULTS					
Component	Requested Concentration	Actual Concentration	Protocol Method	Total Relative Uncertainty	Assay Dates
NOX	100.0 PPM	100.4 PPM	G1	+/- 0.9% NIST Traceable	06/27/2023, 07/06/2023
NITRIC OXIDE	100.0 PPM	100.2 PPM	G1	+/- 0.9% NIST Traceable	06/27/2023, 07/06/2023
SULFUR DIOXIDE	100.0 PPM	100.0 PPM	G1	+/- 1.4% NIST Traceable	06/27/2023, 07/06/2023
CARBON MONOXIDE	200.0 PPM	199.2 PPM	G1	+/- 0.3% NIST Traceable	06/26/2023
CARBON DIOXIDE	8.000 %	7.982 %	G1	+/- 1.2% NIST Traceable	06/27/2023
NITROGEN	Balance				

CALIBRATION STANDARDS					
Type	Lot ID	Cylinder No	Concentration	Uncertainty	Expiration Date
GMIS	104202308	CC754364	98.36 PPM NITRIC OXIDE/NITROGEN	+/- 0.4%	Jan 04, 2031
PRM	C2219101	APE1514048	100.19 PPM NITRIC OXIDE/NITROGEN	+/- 0.3%	Feb 28, 2025
GMIS	2023042525	CC754381	98.52 PPM NITRIC OXIDE/NITROGEN	+/-0.4%	Apr 25, 2031
PRM	12409	D913660	15.01 PPM NITROGEN DIOXIDE/AIR	+/- 1.5%	Feb 17, 2023
GMIS	153400202002	EB0130037	9.693 PPM NITROGEN DIOXIDE/NITROGEN	+/- 1.6%	Sep 29, 2025
NTRM	160102-22	KAL003820	97.69 PPM SULFUR DIOXIDE/NITROGEN	+/- 0.8%	Nov 01, 2027
CO	230601	CC745902	249.47 PPM CARBON MONOXIDE/NITROGEN	+/- 0.3%	Dec 09, 2028
NTRM	130606-02	CC4117130	13.359 % CARBON DIOXIDE/NITROGEN	+/- 0.6%	May 14, 2025
The SRM, NTRM, PRM, or RGM noted above is only in reference to the GMIS used in the assay and not part of the analysis.					

ANALYTICAL EQUIPMENT			
Instrument/Make/Model	Analytical Principle	Last Multipoint Calibration	
Nicolet iS50 FTIR AUP2010245 CO2	FTIR	Jun 15, 2023	
SIEMENS ULTRAMAT6E N1-C8-180	NDIR	Jun 14, 2023	
Nicolet iS50 FTIR AUP2010245 NO	FTIR	Jun 29, 2023	
Nicolet iS50 FTIR AUP2010245 NOX	FTIR	Jun 15, 2023	
Nicolet iS50 FTIR AUP2010245 SO2	FTIR	Jun 08, 2023	

Page 1 of 1

เอกสารไม่ควบคุม

## MULTI-POINT GAS TEST REPORT

Test Date : Sep 6, 2024

Equipment : Gas Analyzer (SO<sub>2</sub>)      Model : 43i  
Manufacturer : Thermo SCIENTIFIC      Serial Number : 1182920016


Standard Gas Concentration			Dilutor Detail	
Sulphur Dioxide (SO <sub>2</sub> )	42.89	PPM	Manufacturer :	Thermo SCIENTIFIC
Nitric Oxide (NO)	46.77	PPM	Model :	146i
Methane (CH <sub>4</sub> )	-	PPM	Serial Number :	1180540071
Carbon Monoxide (CO)	965.9			
Cylinder No. :	EB01159156			
Expiration Date :	Nov 06, 2026			

## Multi-point gas test data

Reference Value (ppb)		Analyzer Display (ppb)	Difference Error	Percent Error	[% Error]
Level 1	Zero	0.0	0.00	0.00	0.00
Level 2	20.00%	100.0	100.3	0.30	0.30
Level 3	40.00%	200.0	200.8	0.80	0.40
Level 4	60.00%	300.0	300.7	0.70	0.23
Level 5	80.00%	400.0	400.0	0.00	0.00

Remark : Measuring Range : 500.0 ppb  
:Acceptable Limit  $\pm$  5%

Average Difference (%) : 0.19

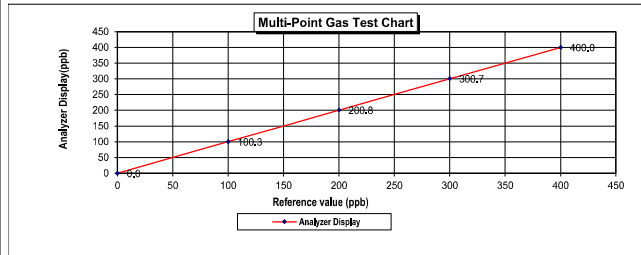

6 / 09 / 2567

6 Sep 2024

Page 1 of 1

เอกสารไม่ควบคุม

## MULTI-POINT GAS TEST REPORT

Test Date : May 15, 2024

Equipment : Gas Analyzer (SO<sub>2</sub>)      Model : 43i  
Manufacturer : Thermo SCIENTIFIC      Serial Number : 1182920017


Standard Gas Concentration			Dilutor Detail	
Sulphur Dioxide (SO <sub>2</sub> )	42.89	PPM	Manufacturer :	Thermo SCIENTIFIC
Nitric Oxide (NO)	46.77	PPM	Model :	146i
Methane (CH <sub>4</sub> )	-	PPM	Serial Number :	1180540071
Carbon Monoxide (CO)	965.9			
Cylinder No. :	EB01159156			
Expiration Date :	Nov 06, 2026			

## Multi-point gas test data

Reference Value (ppb)		Analyzer Display (ppb)	Difference Error	Percent Error	[% Error]
Level 1	Zero	0.0	0.00	0.00	0.00
Level 2	20.00%	100.0	101.7	1.70	1.67
Level 3	40.00%	200.0	200.6	0.60	0.30
Level 4	60.00%	300.0	300.9	0.90	0.30
Level 5	80.00%	400.0	400.0	0.00	0.00

Remark : Measuring Range : 500.0 ppb  
:Acceptable Limit  $\pm$  5%

Average Difference (%) : 0.45

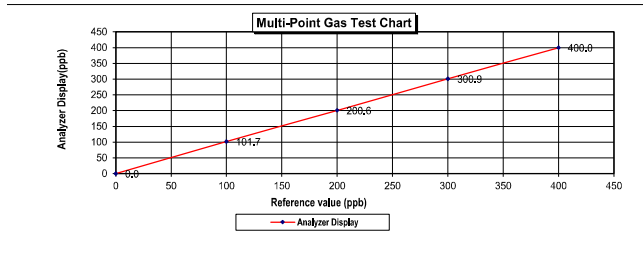

15 / 05 / 2567

15 May 2024

Page 1 of 1

เอกสารไม่ควบคุม

## MULTI-POINT GAS TEST REPORT

Test Date : May 15, 2024

Equipment : Gas Analyzer (SO<sub>2</sub>)      Model : 43i  
Manufacturer : Thermo SCIENTIFIC      Serial Number : 1182920017


Standard Gas Concentration			Dilutor Detail	
Sulphur Dioxide (SO <sub>2</sub> )	42.89	PPM	Manufacturer :	Thermo SCIENTIFIC
Nitric Oxide (NO)	46.77	PPM	Model :	146i
Methane (CH <sub>4</sub> )	-	PPM	Serial Number :	1180540071
Carbon Monoxide (CO)	965.9			
Cylinder No. :	EB01159156			
Expiration Date :	Nov 06, 2026			

## Multi-point gas test data

Reference Value (ppb)		Analyzer Display (ppb)	Difference Error	Percent Error	[% Error]
Level 1	Zero	0.0	0.00	0.00	0.00
Level 2	20.00%	100.0	101.7	1.70	1.67
Level 3	40.00%	200.0	200.6	0.60	0.30
Level 4	60.00%	300.0	300.9	0.90	0.30
Level 5	80.00%	400.0	400.0	0.00	0.00

Remark : Measuring Range : 500.0 ppb  
:Acceptable Limit  $\pm$  5%

Average Difference (%) : 0.45

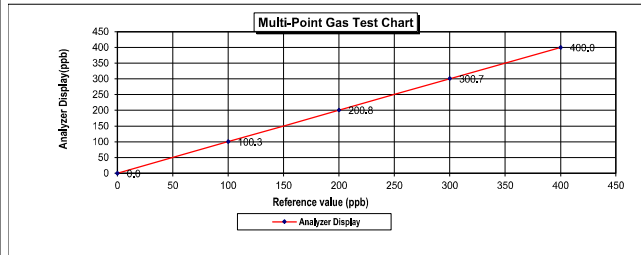

15 / 05 / 2567

15 May 2024

Page 1 of 1

เอกสารไม่ควบคุม

## CERTIFICATE OF ANALYSIS

## Grade of Product: EPA PROTOCOL STANDARD

Customer: AIR LIQUIDE (THAILAND)  
LTD--  
Part Number: E05NI91E15A0014  
Cylinder Number: EB0162121  
Laboratory: 124 - Plumsteadville - PA  
PGVP Number: A12023  
Gas Code: CO, CO2, NO, NOX, SO2, BALN

Reference Number: 160-402772205-1  
Cylinder Volume: 144.0 CF  
Cylinder Pressure: 2016 PSIG  
Valve Outlet: 660  
Certification Date: Jul 06, 2023

Expiration Date: Jul 06, 2031

Certification performed in accordance with "EPA Traceability Protocol for Assay and Certification of Gaseous Calibration Standards (May 2012)" document EPA 800/R-12/531, using the assay procedures listed. Analytical Methodology does not require correction for analytical interference. This cylinder has a total analytical uncertainty as stated below with a confidence level of 95%. There are no significant impurities which affect the use of this calibration mixture. All concentrations are on a mole/mole basis unless otherwise noted. The results relate only to the items tested. The report shall not be reproduced except in full without approval of the laboratory. Do Not Use This Cylinder below 100 psig, i.e. 0.7 megapascals.

ANALYTICAL RESULTS					
Component	Requested Concentration	Actual Concentration	Protocol Method	Total Relative Uncertainty	Assay Dates
NOX	100.0 PPM	100.4 PPM	G1	+/- 0.9% NIST Traceable	06/27/2023, 07/06/2023
NITRIC OXIDE	100.0 PPM	100.2 PPM	G1	+/- 0.9% NIST Traceable	06/27/2023, 07/06/2023
SULFUR DIOXIDE	100.0 PPM	100.0 PPM	G1	+/- 1.4% NIST Traceable	06/27/2023, 07/06/2023
CARBON MONOXIDE	200.0 PPM	199.2 PPM	G1	+/- 0.3% NIST Traceable	06/26/2023
CARBON DIOXIDE	8.000 %	7.982 %	G1	+/- 1.2% NIST Traceable	06/27/2023
NITROGEN	Balance				

CALIBRATION STANDARDS					
Type	Lot ID	Cylinder No	Concentration	Uncertainty	Expiration Date
GMIS	104202308	CC754364	98.36 PPM NITRIC OXIDE/NITROGEN	+/- 0.4%	Jan 04, 2031
PRM	C2219101	APE1514048	100.19 PPM NITRIC OXIDE/NITROGEN	+/- 0.3%	Feb 28, 2025
GMIS	2023042525	CC754381	98.52 PPM NITRIC OXIDE/NITROGEN	+/- 0.4%	Apr 25, 2031
PRM	12409	D913660	15.01 PPM NITROGEN DIOXIDE/AIR	+/- 1.5%	Feb 17, 2023
GMIS	153400202002	EB0130037	9.693 PPM NITROGEN DIOXIDE/NITROGEN	+/- 1.6%	Sep 29, 2025
NTRM	160102-22	KAL003820	97.69 PPM SULFUR DIOXIDE/NITROGEN	+/- 0.8%	Nov 01, 2027
CO	230601	CC745902	249.47 PPM CARBON MONOXIDE/NITROGEN	+/- 0.3%	Dec 09, 2028
NTRM	130606-02	CC411730	13.359 % CARBON DIOXIDE/NITROGEN	+/- 0.6%	May 14, 2025
The SRM, NTRM, PRM, or RGM noted above is only in reference to the GMIS used in the assay and not part of the analysis.					

ANALYTICAL EQUIPMENT			
Instrument/Make/Model	Analytical Principle	Last Multipoint Calibration	
Nicolet iS50 FTIR AUP2010245 CO2	FTIR	Jun 15, 2023	
SIEMENS ULTRAMAT6E N1-C8-180	NDIR	Jun 14, 2023	
Nicolet iS50 FTIR AUP2010245 NO	FTIR	Jun 29, 2023	
Nicolet iS50 FTIR AUP2010245 NOX	FTIR	Jun 15, 2023	
Nicolet iS50 FTIR AUP2010245 SO2	FTIR	Jun 08, 2023	

Page 1 of 1

เอกสารไม่ควบคุม

## MULTI-POINT GAS TEST REPORT

Test Date : Sep 6, 2024

Equipment : Gas Analyzer (SO<sub>2</sub>) Model : 43i  
Manufacturer : Thermo SCIENTIFIC Serial Number : 1182920016


Standard Gas Concentration			Dilutor Detail	
Sulphur Dioxide (SO <sub>2</sub> )	42.89	PPM	Manufacturer :	Thermo SCIENTIFIC
Nitric Oxide (NO)	46.77	PPM	Model :	146i
Methane (CH <sub>4</sub> )	-	PPM	Serial Number :	1180540071
Carbon Monoxide (CO)	965.9			
Cylinder No. :	EB01159156			
Expiration Date :	Nov 06, 2026			

## Multi-point gas test data

Reference Value (ppb)		Analyzer Display (ppb)	Difference Error	Percent Error	[% Error]
Level 1	Zero	0.0	0.00	0.00	0.00
Level 2	20.00%	100.0	100.3	0.30	0.30
Level 3	40.00%	200.0	200.8	0.80	0.40
Level 4	60.00%	300.0	300.7	0.70	0.23
Level 5	80.00%	400.0	400.0	0.00	0.00

Remark : Measuring Range : 500.0 ppb  
:Acceptable Limit  $\pm$  5%

Average Difference (%) : 0.19

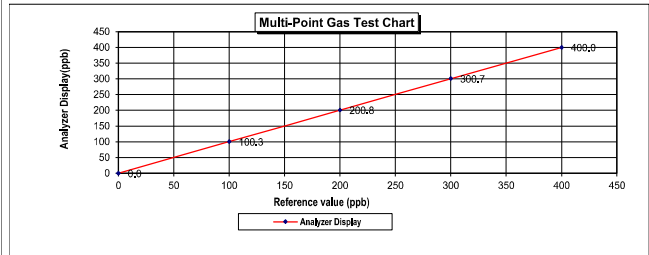

6 9 2567

6 Sep 2024

Page 1 of 1

เอกสารไม่ควบคุม

## MULTI-POINT GAS TEST REPORT

Test Date : May 15, 2024

Equipment : Gas Analyzer (SO<sub>2</sub>) Model : 43i  
Manufacturer : Thermo SCIENTIFIC Serial Number : 1182920017


Standard Gas Concentration			Dilutor Detail	
Sulphur Dioxide (SO <sub>2</sub> )	42.89	PPM	Manufacturer :	Thermo SCIENTIFIC
Nitric Oxide (NO)	46.77	PPM	Model :	146i
Methane (CH <sub>4</sub> )	-	PPM	Serial Number :	1180540071
Carbon Monoxide (CO)	965.9			
Cylinder No. :	EB01159156			
Expiration Date :	Nov 06, 2026			

## Multi-point gas test data

Reference Value (ppb)		Analyzer Display (ppb)	Difference Error	Percent Error	[% Error]
Level 1	Zero	0.0	0.00	0.00	0.00
Level 2	20.00%	100.0	101.7	1.70	1.67
Level 3	40.00%	200.0	200.6	0.60	0.30
Level 4	60.00%	300.0	300.9	0.90	0.30
Level 5	80.00%	400.0	400.0	0.00	0.00

Remark : Measuring Range : 500.0 ppb  
:Acceptable Limit  $\pm$  5%

Average Difference (%) : 0.45

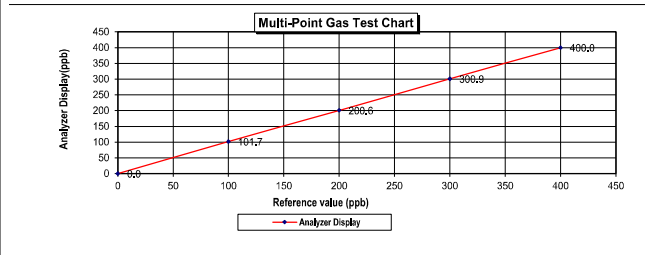

15 '05 2567

15 May 2024

Page 1 of 1

เอกสารไม่ควบคุม

## MULTI-POINT GAS TEST REPORT

Test Date : May 15, 2024

Equipment : Gas Analyzer (SO<sub>2</sub>) Model : 43i  
Manufacturer : Thermo SCIENTIFIC Serial Number : 1182920017


Standard Gas Concentration			Dilutor Detail	
Sulphur Dioxide (SO <sub>2</sub> )	42.89	PPM	Manufacturer :	Thermo SCIENTIFIC
Nitric Oxide (NO)	46.77	PPM	Model :	146i
Methane (CH <sub>4</sub> )	-	PPM	Serial Number :	1180540071
Carbon Monoxide (CO)	965.9			
Cylinder No. :	EB01159156			
Expiration Date :	Nov 06, 2026			

## Multi-point gas test data

Reference Value (ppb)		Analyzer Display (ppb)	Difference Error	Percent Error	[% Error]
Level 1	Zero	0.0	0.00	0.00	0.00
Level 2	20.00%	100.0	101.7	1.70	1.67
Level 3	40.00%	200.0	200.6	0.60	0.30
Level 4	60.00%	300.0	300.9	0.90	0.30
Level 5	80.00%	400.0	400.0	0.00	0.00

Remark : Measuring Range : 500.0 ppb  
:Acceptable Limit  $\pm$  5%

Average Difference (%) : 0.45

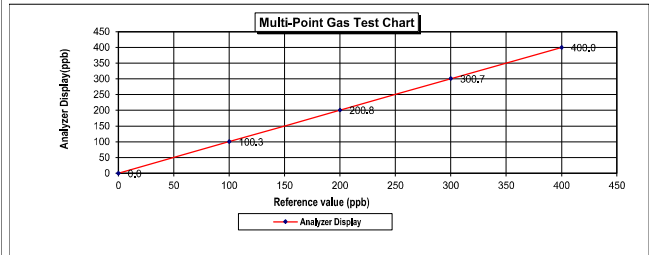

15 '05 2567

15 May 2024

Page 1 of 1

เอกสารไม่ควบคุม

MULTI-POINT GAS TEST REPORT


Test Date : Sep 4, 2024

Equipment : Gas Analyzer (SO<sub>2</sub>) Model : 43i  
Manufacturer : Thermo SCIENTIFIC Serial Number : 1180540065

Standard Gas Concentration			Dilutor Detail	
Sulphur Dioxide (SO <sub>2</sub> )	42.89	PPM	Manufacturer :	Thermo SCIENTIFIC
Nitric Oxide (NO)	46.77	PPM	Model :	146i
Methane (CH <sub>4</sub> )	-	PPM	Serial Number :	1180540071
Carbon Monoxide (CO)	965.9			
Cylinder No. :	EB01159156			
Expiration Date :	Nov 06, 2026			

Multi-point gas test data

Reference Value (ppb)			Analyzer Display (ppb)	Difference Error	Percent Error	[% Error ]
Level 1	Zero	0.0	0.0	0.00	0.00	0.00
Level 2	20.00%	100.0	100.7	0.70	0.70	0.70
Level 3	40.00%	200.0	200.4	0.40	0.20	0.20
Level 4	60.00%	300.0	300.8	0.80	0.27	0.27
Level 5	80.00%	400.0	400.0	0.00	0.00	0.00
Remark : Measuring Range			500.0 ppb		Average Difference (%) 0.23	

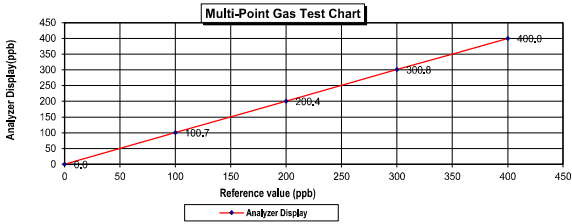

4 / 9 / 2567  
4 / Sep / 2024

CERTIFICATE OF ANALYSIS

Grade of Product: EPA PROTOCOL STANDARD

Customer: AIR LIQUIDE (THAILAND)  
LTD:-  
Part Number: E05NI91E15A0014 Reference Number: 160-402772205-1  
Cylinder Number: EB0162121 Cylinder Volume: 144.0 CF  
Laboratory: 124 - Plumsteadville - PA Cylinder Pressure: 2016 PSIG  
PGVP Number: A12023 Valve Outlet: 660  
Gas Code: CO, CO<sub>2</sub>, NO, NOX, SO<sub>2</sub>, BALN Certification Date: Jul 06, 2023  
Expiration Date: Jul 06, 2031

Certification performed in accordance with "EPA Traceability Protocol for Assay and Certification of Gaseous Calibration Standards (May 2012)" document EPA 800/R-12/531, using the assay procedures listed. Analytical Methodology does not require correction for analytical interference. This cylinder has a total analytical uncertainty as stated below with a confidence level of 95%. There are no significant impurities which affect the use of this calibration mixture. All concentrations are on a mole/mole basis unless otherwise noted. The results relate only to the items listed. The report shall not be reproduced except in full without approval of the laboratory. Do Not Use This Cylinder below 100 psig, i.e. 0.7 megapascals.

ANALYTICAL RESULTS					
Component	Requested Concentration	Actual Concentration	Protocol Method	Total Relative Uncertainty	Assay Dates
NOX	100.0 PPM	100.4 PPM	G1	+/- 0.9% NIST Traceable	06/27/2023, 07/06/2023
NITRIC OXIDE	100.0 PPM	100.2 PPM	G1	+/- 0.9% NIST Traceable	06/27/2023, 07/06/2023
SULFUR DIOXIDE	100.0 PPM	100.0 PPM	G1	+/- 1.4% NIST Traceable	06/27/2023, 07/06/2023
CARBON MONOXIDE	200.0 PPM	199.2 PPM	G1	+/- 0.3% NIST Traceable	06/26/2023
CARBON DIOXIDE	8.000 %	7.982 %	G1	+/- 1.2% NIST Traceable	06/27/2023
NITROGEN	Balance				

CALIBRATION STANDARDS					
Type	Lot ID	Cylinder No	Concentration	Uncertainty	Expiration Date
GMIS	104202308	CC754364	98.36 PPM NITRIC OXIDE/NITROGEN	+/- 0.4%	Jan 04, 2031
PRM	C2219101	AP1514048	100.19 PPM NITRIC OXIDE/NITROGEN	+/- 0.3%	Feb 28, 2025
GMIS	2023042525	CC754381	98.52 PPM NITRIC OXIDE/NITROGEN	+/- 0.4%	Apr 25, 2031
PRM	12409	D913660	15.01 PPM NITROGEN DIOXIDE/AIR	+/- 1.5%	Feb 17, 2023
GMIS	153400202002	EB0130037	9.693 PPM NITROGEN DIOXIDE/NITROGEN	+/- 1.6%	Sep 29, 2025
NTRM	160102-22	KAL003820	97.69 PPM SULFUR DIOXIDE/NITROGEN	+/- 0.8%	Nov 01, 2027
CO	230601	CC745902	249.47 PPM CARBON MONOXIDE/NITROGEN	+/- 0.3%	Dec 09, 2028
NTRM	130806-02	CC411730	13.359 % CARBON DIOXIDE/NITROGEN	+/- 0.6%	May 14, 2025
The SRM, NTRM, PRM, or RGM noted above is only in reference to the GMIS used in the assay and not part of the analysis.					

ANALYTICAL EQUIPMENT			
Instrument/Make/Model	Analytical Principle	Last Multipoint Calibration	
Nicolet IS50 FTIR AUP2010245 CO2	FTIR	Jun 15, 2023	
SIEMENS ULTRAMAT6E N1-C8-180	NDIR	Jun 14, 2023	
Nicolet IS50 FTIR AUP2010245 NO	FTIR	Jun 29, 2023	
Nicolet IS50 FTIR AUP2010245 NO2	FTIR	Jun 15, 2023	
Nicolet IS50 FTIR AUP2010245 SO2	FTIR	Jun 08, 2023	

Approved for Release

MULTI-POINT GAS TEST REPORT


Test Date : Sep 9, 2024

Equipment : Gas Analyzer (CO) Model : 48i  
Manufacturer : Thermo Scientific Serial Number : 1180540074

Standard Gas Concentration			Dilutor Detail	
Sulphur Dioxide (SO <sub>2</sub> )	42.89	PPM	Manufacturer :	Thermo Scientific
Nitric Oxide (NO)	46.77	PPM	Model :	146i
Methane (CH <sub>4</sub> )	-	PPM	Serial Number :	1180540071
Carbon Monoxide (CO)	965.9	PPM		
Cylinder No. :	EB01159156			
Expiration Date :	Nov 06, 2026			

Multi-point gas test data

Reference Value (ppm)			Analyzer Display (ppm)	Difference Error	Percent Error	[% Error ]
Level 1	Zero	0.0	0.0	0.0	0.0	0.0
Level 2	20.00%	10.0	10.4	0.4	3.8	3.8
Level 3	40.00%	20.0	20.8	0.8	3.8	3.8
Level 4	60.00%	30.0	30.5	0.5	1.6	1.6
Level 5	80.00%	40.0	40.0	0.0	0.0	0.0
Remark : Measuring Range			50.0 ppm	Average Difference (%)		1.87

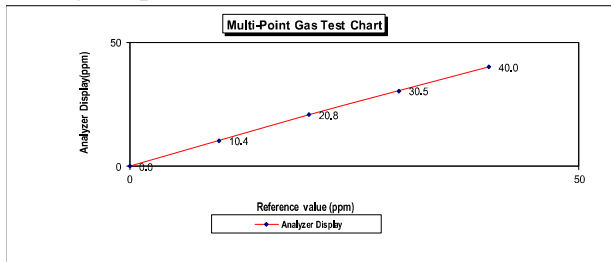

9 / 9 / 2567  
9 / Sep / 2024

MULTI-POINT GAS TEST REPORT


Test Date : June 14, 2024

Equipment : Gas Analyzer (CO) Model : APM4-370  
Manufacturer : HORIBA Serial Number : YN43AG7T

Standard Gas Concentration			Dilutor Detail	
Sulphur Dioxide (SO <sub>2</sub> )	42.89	PPM	Manufacturer :	Thermo Scientific
Nitric Oxide (NO)	46.77	PPM	Model :	146i
Methane (CH <sub>4</sub> )	-	PPM	Serial Number :	1180540071
Carbon Monoxide (CO)	965.9	PPM		
Cylinder No. :	EB01159156			
Expiration Date :	Nov 06, 2026			

Multi-point gas test data

Reference Value (ppm)			Analyzer Display (ppm)	Difference Error	Percent Error	[% Error ]
Level 1	Zero	0.0	0.0	0.0	0.0	0.0
Level 2	20.00%	10.0	10.9	0.9	8.3	8.3
Level 3	40.00%	20.0	20.5	0.5	2.4	2.4
Level 4	60.00%	30.0	30.7	0.7	2.3	2.3
Level 5	80.00%	40.0	40.0	0.0	0.0	0.0
Remark : Measuring Range			50.0 ppm	Average Difference (%)		2.60

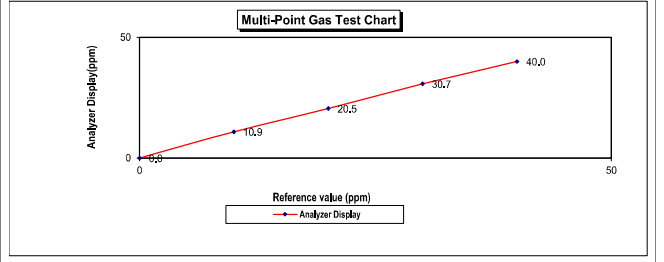

14 / 06 / 2567  
14 / June / 2024

### MULTI-POINT GAS TEST REPORT

Test Date : Sep 3, 2024

Equipment : Gas Analyzer (CO) Model : 48i  
Manufacturer : Thermo Scientific Serial Number : CM08140004

#### Standard Gas Concentration

Sulphur Dioxide (SO<sub>2</sub>) 42.89 PPM  
Nitric Oxide (NO) 46.77 PPM  
Methane (CH<sub>4</sub>) - PPM  
Carbon Monoxide (CO) 965.9 PPM  
Cylinder No. : EB01159156  
Expiration Date : Nov 06, 2026


#### Dilutor Detail

Manufacturer : Thermo Scientific  
Model : 146i  
Serial Number : 1180540071

#### Multi-point gas test data

	Reference Value (ppm)	Analyzer Display (ppm)	Difference Error	Percent Error	[% Error ]
Level 1	Zero	0.0	0.0	0.0	0.0
Level 2	20.00%	10.0	10.5	0.5	4.8
Level 3	40.00%	20.0	20.9	0.9	4.3
Level 4	60.00%	30.0	30.7	0.7	2.3
Level 5	80.00%	40.0	40.0	0.0	0.0

Remark : Measuring Range 50.0 ppm  
:Acceptable Limit ± 5%

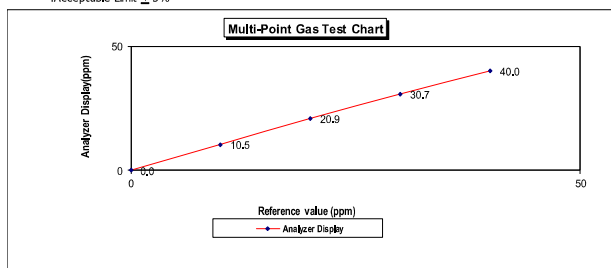

3.....9...../2567

3.....Sep..../2024

Page 1 of 1

เอกสารไม่ควบคุม

### MULTI-POINT GAS TEST REPORT

Test Date : June 14, 2024

Equipment : Gas Analyzer (CO) Model : 48i  
Manufacturer : Thermo Scientific Serial Number : 1182920018

#### Standard Gas Concentration

Sulphur Dioxide (SO<sub>2</sub>) 42.89 PPM  
Nitric Oxide (NO) 46.77 PPM  
Methane (CH<sub>4</sub>) - PPM  
Carbon Monoxide (CO) 965.9 PPM  
Cylinder No. : EB01159156  
Expiration Date : Nov 06, 2026


#### Dilutor Detail

Manufacturer : Thermo Scientific  
Model : 146i  
Serial Number : 1180540071

#### Multi-point gas test data

	Reference Value (ppm)	Analyzer Display (ppm)	Difference Error	Percent Error	[% Error ]
Level 1	Zero	0.0	0.0	0.0	0.0
Level 2	20.00%	10.0	10.7	0.7	6.5
Level 3	40.00%	20.0	20.7	0.7	3.4
Level 4	60.00%	30.0	30.9	0.9	2.9
Level 5	80.00%	40.0	40.0	0.0	0.0

Remark : Measuring Range 50.0 ppm  
:Acceptable Limit ± 5%

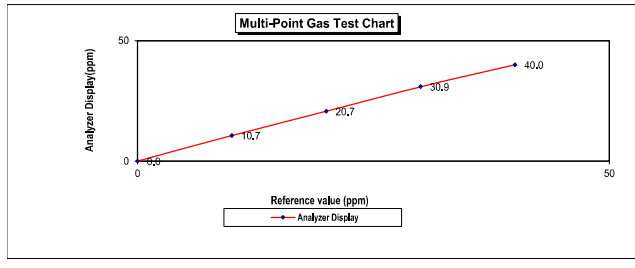

14.....06...../2567

14.....June..../2024

Page 1 of 1

เอกสารไม่ควบคุม



Airgas Specialty Gases  
Airgas USA LLC  
6111 Easton Road  
Plumsteadville, PA 18949  
Airgas.com

## CERTIFICATE OF ANALYSIS

### Grade of Product: EPA PROTOCOL STANDARD

Customer: AIR LIQUIDE (THAILAND)  
LTD--  
Part Number: E05NI91E15A0014 Reference Number: 160-402772205-1  
Cylinder Number: EB0162121 Cylinder Volume: 144.0 CF  
Laboratory: 124 - Plumsteadville - PA Cylinder Pressure: 2016 PSIG  
PGVP Number: A12023 Valve Outlet: 660  
Gas Code: CO, CO<sub>2</sub>, NO, NO<sub>2</sub>, SO<sub>2</sub>, BALN Certification Date: Jul 06, 2023

Expiration Date: Jul 06, 2031

Certification performed in accordance with "EPA Traceability Protocol for Assay and Certification of Gaseous Calibration Standards" (May 2012) document EPA 800R-12/531, using the assay procedures listed. Analytical Methodology does not require correction for analytical interference. This cylinder has a total analytical uncertainty as stated below with a confidence level of 95%. There are no significant impurities which affect the use of this calibration mixture. All concentrations are on a mole/mole basis unless otherwise noted. The results relate only to the items listed. The report shall not be reproduced except in full without approval of the laboratory. Do Not Use This Cylinder below 100 psig, i.e. 0.7 megapascals.

Component	Requested Concentration	Actual Concentration	Protocol Method	Total Relative Uncertainty	Assay Dates
NOX	100.0 PPM	100.4 PPM	G1	+/- 0.9% NIST Traceable	06/27/2023, 07/06/2023
NITRIC OXIDE	100.0 PPM	100.2 PPM	G1	+/- 0.9% NIST Traceable	06/27/2023, 07/06/2023
SULFUR DIOXIDE	100.0 PPM	100.0 PPM	G1	+/- 1.4% NIST Traceable	06/27/2023, 07/06/2023
CARBON MONOXIDE	200.0 PPM	199.2 PPM	G1	+/- 0.3% NIST Traceable	06/26/2023
CARBON DIOXIDE	8.000 %	7.982 %	G1	+/- 1.2% NIST Traceable	06/27/2023
NITROGEN	Balance				

#### CALIBRATION STANDARDS

Type	Lot ID	Cylinder No	Concentration	Uncertainty	Expiration Date
GMIS	104202308	CC754364	98.36 PPM NITRIC OXIDE/NITROGEN	+/- 0.4%	Jan 04, 2031
PRM	C2219101	APE1514048	100.19 PPM NITRIC OXIDE/NITROGEN	+/- 0.3%	Feb 28, 2025
GMIS	2023042525	CC754381	98.52 PPM NITRIC OXIDE/NITROGEN	+/-0.4%	Apr 25, 2031
PRM	12409	D913660	15.01 PPM NITROGEN DIOXIDE/AIR	+/- 1.5%	Feb 17, 2023
GMIS	153400202002	EB0130037	9.693 PPM NITROGEN DIOXIDE/NITROGEN	+/- 1.6%	Sep 29, 2025
NTRM	160102-22	KAL003820	97.69 PPM SULFUR DIOXIDE/NITROGEN	+/- 0.8%	Nov 01, 2027
CO	230601	CC745902	249.47 PPM CARBON MONOXIDE/NITROGEN	+/- 0.3%	Dec 09, 2028
NTRM	130606-02	CC411730	13.359 % CARBON DIOXIDE/NITROGEN	+/- 0.6%	May 14, 2025

The SRM, NTRM, PRM, or RGM noted above is only in reference to the GMIS used in the assay and not part of the analysis.

#### ANALYTICAL EQUIPMENT

Instrument/Make/Model	Analytical Principle	Last Multipoint Calibration
Nicolet iS50 FTIR AUP2010245 CO <sub>2</sub>	FTIR	Jun 15, 2023
SIEMENS ULTRAMAT6E N1-C8-180	NDIR	Jun 14, 2023
Nicolet iS50 FTIR AUP2010245 NO	FTIR	Jun 29, 2023
Nicolet iS50 FTIR AUP2010245 NO <sub>2</sub>	FTIR	Jun 15, 2023
Nicolet iS50 FTIR AUP2010245 SO <sub>2</sub>	FTIR	Jun 08, 2023



## CALIBRATION LABORATORY Co., LTD.

2/10-11, 14, 55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230  
Tel. 02-578-0353-4 Fax. 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



## CERTIFICATE OF CALIBRATION

### FOR

NOMENCLATURE : VIBRATION METER  
MANUFACTURER : INSTANTEL  
MODEL / TYPE : 721A2601/721A3301  
SERIAL NO. : UM11056/UM11056  
CLID. NO. : 252000389  
JOB CONTROL NO. : 240406037351  
CALIBRATION SERVICE : ☒ IN-LABORATORY ☐ ON-SITE

CUSTOMER : UNITED ANALYST AND ENGINEERING CONSULTANT CO., LTD.  
81 SOI UDOMSUK 41, SUKHUMVIT ROAD,  
BANGCHAK, PHRAKHANONG, BANGKOK 10260

DATE OF RECEIVED : 06 April 2024

DATE OF ISSUED : 10 April 2024

The report of calibration shall not be reproduced except in full without approval of the Calibration Laboratory Co., Ltd.

Calibrated By : Suwit Phuanbusabong  
Calibration Engineer

Approved By :  
Authorized Signatory  
10 April 2024

This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to the International System of Units (SI)

Certificate No. Q24037351  
F3-011-05/12-23



เอกสารไม่ควบคุม

เอกสารไม่ควบคุม







# CALIBRATION LABORATORY Co.,LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230  
Tel. 02-578-0353-4 Fax. 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



# CALIBRATION LABORATORY Co.,LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230  
Tel. 02-578-0353-4 Fax. 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



## REPORT OF CALIBRATION

### FOR

NOMENCLATURE : VIBRATION METER  
MANUFACTURER : INSTANTEL  
MODEL / TYPE : 721A2601/721A3301  
SERIAL NO. : UM11056/UM11056  
DATE OF CALIBRATION : 08 April 2024

#### ENVIRONMENT CONDITIONS :

Temperature : (23 ± 2) °C Relative Humidity : (55 ± 15) %RH

#### PROCEDURE USED :

This instrument was calibrated under procedure No. CLC-CPEE-08 based on ISO 16063-21 as calibration guideline.  
The calibration was performed by using Digital Multimeter, Universal Counter, Accelerometer and Measuring Amplifier which maintained by the Calibration Laboratory Co., Ltd.

#### REFERENCE STANDARD USED :

- Digital Multimeter, Wavetek Model 1281 S/N. 29320.
- Universal Counter, Hewlett Packard Model 5315A S/N. 2448A13042.
- Accelerometer with Measuring Amplifier, Bruel & Kjaer Model 8305, 2525 S/N. 397018, 2434988.

#### TRACEABILITY :

- The measurements are traceable to International System of Units (SI), through Aeronautical Radio of Thailand Ltd. Certificate No. 05-0316/23, Due Date 21 July 2025.
- The measurements are traceable to International System of Units (SI), through Aeronautical Radio of Thailand Ltd. Certificate No. 07-0159/23, Due Date 04 December 2024.
- The measurements are traceable to International System of Units (SI), through National Institute of Metrology (Thailand) Certificate No. AV-0052-23, Due Date 26 September 2024.

#### UNCERTAINTY :

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor  $k = 2.00$  which for a normal distribution corresponds to a coverage probability of approximately 95%. It has been evaluated according to the "Evaluation of the Uncertainty of Measurement in Calibration (EA-4/02 M:2022)"

Certificate No. Q24037351

F3-011-05/12-23

page 2 of 4

เอกสารไม่ควบคุม



@clccalibration

CONDITION OF CALIBRATION ITEM : RECEIVED IN GOOD OPERATIONAL CONDITION

MEASUREMENT RESULTS : (X) without adjustment ( ) adjustment

#### CALIBRATION DATA

##### 1. ACCELERATION RESULT

Test point		Mode	STD Reading	DUC Reading	Correction	Uncertainty
(g)	(frequency)		(g)	(g)	(g)	± (% of rdg.)
0.3	50 Hz	peak	0.300	0.302	-0.002	1.9
0.4	50 Hz		0.400	0.404	-0.004	1.6
0.5	50 Hz		0.500	0.505	-0.005	1.6
0.6	50 Hz		0.600	0.607	-0.007	2.5
0.7	50 Hz		0.700	0.708	-0.008	2.5
0.3	100 Hz	peak	0.300	0.302	-0.002	1.9
0.4	100 Hz		0.400	0.403	-0.003	1.6
0.5	100 Hz		0.500	0.505	-0.005	1.6
0.6	100 Hz		0.600	0.607	-0.007	2.5
0.7	100 Hz		0.700	0.708	-0.008	2.5

##### 2. VELOCITY RESULT

Test point		Mode	STD Reading	DUC Reading	Correction	Uncertainty
(mm/s)	(frequency)		(mm/s)	(mm/s)	(mm/s)	± (% of rdg.)
3	50 Hz	peak	3.000	3.048	-0.048	1.8
4	50 Hz		4.000	4.058	-0.058	1.8
5	50 Hz		5.000	5.066	-0.066	1.8
6	50 Hz		6.000	6.079	-0.079	1.8
7	50 Hz		7.000	7.089	-0.089	1.8
*3	100 Hz	peak	3.000	3.033	-0.033	1.6
*4	100 Hz		4.000	4.045	-0.045	1.6
*5	100 Hz		5.000	5.056	-0.056	1.6
*6	100 Hz		6.000	6.067	-0.067	1.5
*7	100 Hz		7.000	7.079	-0.079	1.5

Certificate No. Q24037351

F3-011-05/12-23

page 3 of 4

เอกสารไม่ควบคุม



@clccalibration



# CALIBRATION LABORATORY Co.,LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230  
Tel. 02-578-0353-4 Fax. 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



# CALIBRATION LABORATORY Co.,LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230  
Tel. 02-578-0353-4 Fax. 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



#### CALIBRATION DATA

##### 3. DISPLACEMENT RESULT

Test point		Mode	STD Reading	DUC Reading	Correction	Uncertainty
(mm)	(frequency)		(mm)	(mm)	(mm)	± (% of rdg.)
0.03	50 Hz	peak	0.030	0.030	0.000	2.5
0.04	50 Hz		0.040	0.040	0.000	2.1
0.05	50 Hz		0.050	0.050	0.000	1.9
0.06	50 Hz		0.060	0.061	-0.001	1.8
0.07	50 Hz		0.070	0.071	-0.001	1.8
0.03	100 Hz	peak	0.030	0.030	0.000	2.5
0.04	100 Hz		0.040	0.040	0.000	2.1
0.05	100 Hz		0.050	0.050	0.000	1.9
0.06	100 Hz		0.060	0.061	-0.001	1.8
0.07	100 Hz		0.070	0.071	-0.001	1.8

Note. The Scope of Accredited ANAB Certificate No. ACDM-2814 Version 012 Page 1,2 of 67

\* means Calibrations marked "Not ANAB Accredited" in this Certificate have been included for completeness.

This report is valid for the above stated instrument/s only.

### End of Certificate ###

## CERTIFICATE OF CALIBRATION

### FOR

NOMENCLATURE : VIBRATION METER  
MANUFACTURER : INSTANTEL  
MODEL / TYPE : 721A2601/721A3301  
SERIAL NO. : UM11057/UM11057  
CLID. NO. : 252000248  
JOB CONTROL NO. : 240429042939  
CALIBRATION SERVICE : ☒ IN-LABORATORY ☐ ON-SITE

CUSTOMER : UNITED ANALYST AND ENGINEERING CONSULTANT CO., LTD.

81 SOI UDOMSUK 41, SUKHUMVIT ROAD,  
BANGCHAK, PHRAKHANONG, BANGKOK 10260

DATE OF RECEIVED : 29 April 2024

DATE OF ISSUED : 03 May 2024

The report of calibration shall not be reproduced except in full without approval of the Calibration Laboratory Co., Ltd.

Calibrated By : Suwit Phuanbusabong  
Calibration Engineer



Approved By :

Authorized Signatory  
03 May 2024

This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to the International System of Units (SI)

Certificate No. Q24037351

F3-011-05/12-23

page 4 of 4

เอกสารไม่ควบคุม



@clccalibration

Certificate No. Q24042939

F3-011-05/12-23

page 1 of 4

เอกสารไม่ควบคุม



@clccalibration





# CALIBRATION LABORATORY Co., LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230  
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cai-laboratory.com E-mail:sale@cai-laboratory.com



# CALIBRATION LABORATORY Co., LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230  
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cai-laboratory.com E-mail:sale@cai-laboratory.com



## REPORT OF CALIBRATION

### FOR

NOMENCLATURE : VIBRATION METER  
MANUFACTURER : INSTANTEL  
MODEL / TYPE : 721A2601/721A3301  
SERIAL NO. : UM11057/UM11057  
DATE OF CALIBRATION : 30 April 2024

#### ENVIRONMENT CONDITIONS :

Temperature : (23 ± 2) °C Relative Humidity : (55 ± 15) %RH

#### PROCEDURE USED :

This instrument was calibrated under procedure No. CLC-CPEE-08 based on ISO 16063-21 as calibration guideline.

The calibration was performed by using Digital Multimeter, Universal Counter,

Accelerometer and Measuring Amplifier which maintained by the Calibration Laboratory Co., Ltd.

#### REFERENCE STANDARD USED :

1. Digital Multimeter, Wavetek Model 1281 S/N. 29320.
2. Universal Counter, Hewlett Packard Model 5315A S/N. 2448A13042.
3. Accelerometer with Measuring Amplifier, Bruel & Kjaer Model 8305, 2525 S/N. 397018, 2434988.

#### TRACEABILITY :

1. The measurements are traceable to International System of Units (SI), through Aeronautical Radio of Thailand Ltd. Certificate No. 05-0316/23, Due Date 21 July 2025.
2. The measurements are traceable to International System of Units (SI), through Aeronautical Radio of Thailand Ltd. Certificate No. 07-0159/23, Due Date 04 December 2024.
3. The measurements are traceable to International System of Units (SI), through National Institute of Metrology (Thailand) Certificate No. AV-0052-23, Due Date 26 September 2024.

#### UNCERTAINTY :

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor  $k = 2.00$  which for a normal distribution corresponds to a coverage probability of approximately 95 %.

It has been evaluated according to the "Evaluation of the Uncertainty of Measurement in Calibration (EA-4/02 M:2022)"

Certificate No. Q24042939

F3-011-05/12-23

page 2 of 4

เอกสารไม่ควบคุม



@clccalibration

CONDITION OF CALIBRATION ITEM : RECEIVED IN GOOD OPERATIONAL CONDITION

MEASUREMENT RESULTS : ( X ) without adjustment ( ) adjustment

#### CALIBRATION DATA

##### 1. ACCELERATION RESULT

Test point		Mode	STD Reading	DUC Reading	Correction	Uncertainty
( g )	( frequency )		( g )	( g )	( g )	± ( % of rdg. )
0.3	50 Hz	peak	0.300	0.304	-0.004	1.9
0.4	50 Hz		0.400	0.406	-0.006	1.6
0.5	50 Hz		0.500	0.507	-0.007	1.6
0.6	50 Hz		0.600	0.608	-0.008	2.5
0.7	50 Hz		0.700	0.709	-0.009	2.5
0.3	100 Hz	peak	0.300	0.305	-0.005	1.9
0.4	100 Hz		0.400	0.407	-0.007	1.6
0.5	100 Hz		0.500	0.508	-0.008	1.6
0.6	100 Hz		0.600	0.609	-0.009	2.5
0.7	100 Hz		0.700	0.711	-0.011	2.5

##### 2. VELOCITY RESULT

Test point		Mode	STD Reading	DUC Reading	Correction	Uncertainty
( mm/s )	( frequency )		( mm/s )	( mm/s )	( mm/s )	± ( % of rdg. )
3	50 Hz	peak	3.000	3.036	-0.036	1.8
4	50 Hz		4.000	4.047	-0.047	1.8
5	50 Hz		5.000	5.059	-0.059	1.8
6	50 Hz		6.000	6.069	-0.069	1.8
7	50 Hz		7.000	7.083	-0.083	1.8
*3	100 Hz	peak	3.000	3.045	-0.045	1.6
*4	100 Hz		4.000	4.054	-0.054	1.6
*5	100 Hz		5.000	5.063	-0.063	1.6
*6	100 Hz		6.000	6.076	-0.076	1.5
*7	100 Hz		7.000	7.088	-0.088	1.5

Certificate No. Q24042939

F3-011-05/12-23

page 3 of 4

เอกสารไม่ควบคุม



@clccalibration



# CALIBRATION LABORATORY Co., LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230  
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cai-laboratory.com E-mail:sale@cai-laboratory.com



# CALIBRATION LABORATORY Co., LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230  
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cai-laboratory.com E-mail:sale@cai-laboratory.com



#### CALIBRATION DATA

##### 3. DISPLACEMENT RESULT

Test point		Mode	STD Reading	DUC Reading	Correction	Uncertainty
( mm )	( frequency )		( mm )	( mm )	( mm )	± ( % of rdg. )
0.03	50 Hz	peak	0.030	0.030	0.000	2.5
0.04	50 Hz		0.040	0.040	0.000	2.1
0.05	50 Hz		0.050	0.050	0.000	1.9
0.06	50 Hz		0.060	0.061	-0.001	1.8
0.07	50 Hz		0.070	0.071	-0.001	1.8
0.03	100 Hz	peak	0.030	0.030	0.000	2.5
0.04	100 Hz		0.040	0.040	0.000	2.1
0.05	100 Hz		0.050	0.050	0.000	1.9
0.06	100 Hz		0.060	0.061	-0.001	1.8
0.07	100 Hz		0.070	0.071	-0.001	1.8

Note: The Scope of Accredited ANAB Certificate No. ACDM-2814 Version 012 Page 1,2 of 67

\* means Calibrations marked " Not ANAB Accredited " in this Certificate have been included for completeness.

This report is valid for the above stated instrument/s only.

### End of Certificate ###

Certificate No. Q24042939

F3-011-05/12-23

page 4 of 4

เอกสารไม่ควบคุม



@clccalibration

## CERTIFICATE OF CALIBRATION

### FOR

NOMENCLATURE : VIBRATION METER  
MANUFACTURER : INSTANTEL  
MODEL / TYPE : 721A2601/721A3301  
SERIAL NO. : UM11058/UM11058  
CLID. NO. : 252000350  
JOB CONTROL NO. : 240406037354  
CALIBRATION SERVICE : ☒ IN-LABORATORY ☐ ON-SITE

CUSTOMER : UNITED ANALYST AND ENGINEERING CONSULTANT CO., LTD.

81 SOI UDOSUK 41, SUKHUMVIT ROAD,  
BANGCHAK, PHRAKHANONG, BANGKOK 10260

DATE OF RECEIVED : 06 April 2024

DATE OF ISSUED : 10 April 2024

The report of calibration shall not be reproduced except in full without approval of the Calibration Laboratory Co., Ltd.

Calibrated By :

Suwit Phuanbusabong  
Calibration Engineer

Approved By :

Authorized Signatory  
10 April 2024

This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to the International System of Units ( SI )

Certificate No. Q24037354

F3-011-05/12-23

page 1 of 4

เอกสารไม่ควบคุม



@clccalibration



# CALIBRATION LABORATORY Co.,LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230  
Tel. 02-578-0353-4 Fax. 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



# CALIBRATION LABORATORY Co.,LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230  
Tel. 02-578-0353-4 Fax. 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



## REPORT OF CALIBRATION

### FOR

NOMENCLATURE : VIBRATION METER  
MANUFACTURER : INSTANTEL  
MODEL / TYPE : 721A2601/721A3301  
SERIAL NO. : UM11058/UM11058  
DATE OF CALIBRATION : 08 April 2024

#### ENVIRONMENT CONDITIONS :

Temperature : (23 ± 2) °C Relative Humidity : (55 ± 15) %RH

#### PROCEDURE USED :

This instrument was calibrated under procedure No. CLC-CPEE-08 based on ISO 16063-21 as calibration guideline.  
The calibration was performed by using Digital Multimeter, Universal Counter,  
Accelerometer and Measuring Amplifier which maintained by the Calibration Laboratory Co., Ltd.

#### REFERENCE STANDARD USED :

- Digital Multimeter, Wavetek Model 1281 S/N. 29320.
- Universal Counter, Hewlett Packard Model 5315A S/N. 2448A13042.
- Accelerometer with Measuring Amplifier, Bruel & Kjaer Model 8305, 2525 S/N. 397018, 2434988.

#### TRACEABILITY :

- The measurements are traceable to International System of Units (SI), through Aeronautical Radio of Thailand Ltd.  
Certificate No. 05-0316/23, Due Date 21 July 2025.
- The measurements are traceable to International System of Units (SI), through Aeronautical Radio of Thailand Ltd.  
Certificate No. 07-0159/23, Due Date 04 December 2024.
- The measurements are traceable to International System of Units (SI), through National Institute of Metrology (Thailand)  
Certificate No. AV-0052-23, Due Date 26 September 2024.

#### UNCERTAINTY :

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied  
by the coverage factor  $k = 2.00$  which for a normal distribution corresponds to a coverage probability of approximately 95 %.  
It has been evaluated according to the "Evaluation of the Uncertainty of Measurement in Calibration (EA-4/02 M:2022)"

Certificate No. Q24037354

F3-011-05/12-23

page 2 of 4

เอกสารไม่ควบคุม



@clccalibration

CONDITION OF CALIBRATION ITEM : RECEIVED IN GOOD OPERATIONAL CONDITION

MEASUREMENT RESULTS : (X) without adjustment ( ) adjustment

#### CALIBRATION DATA

##### 1. ACCELERATION RESULT

Test point		Mode	STD Reading	DUC Reading	Correction	Uncertainty
(g)	(frequency)		(g)	(g)	(g)	± (% of rdg.)
0.3	50 Hz	peak	0.300	0.295	+0.005	1.9
0.4	50 Hz		0.400	0.394	+0.006	1.6
0.5	50 Hz		0.500	0.493	+0.007	1.6
0.6	50 Hz		0.600	0.593	+0.007	2.5
0.7	50 Hz		0.700	0.692	+0.008	2.5
0.3	100 Hz	peak	0.300	0.296	+0.004	1.9
0.4	100 Hz		0.400	0.395	+0.005	1.6
0.5	100 Hz		0.500	0.494	+0.006	1.6
0.6	100 Hz		0.600	0.594	+0.006	2.5
0.7	100 Hz		0.700	0.693	+0.007	2.5

##### 2. VELOCITY RESULT

Test point		Mode	STD Reading	DUC Reading	Correction	Uncertainty
(mm/s)	(frequency)		(mm/s)	(mm/s)	(mm/s)	± (% of rdg.)
3	50 Hz	peak	3.000	2.989	+0.011	1.8
4	50 Hz		4.000	3.981	+0.019	1.8
5	50 Hz		5.000	4.962	+0.038	1.8
6	50 Hz		6.000	5.939	+0.061	1.8
7	50 Hz		7.000	6.924	+0.076	1.8
*3	100 Hz	peak	3.000	2.983	+0.017	1.6
*4	100 Hz		4.000	3.972	+0.028	1.6
*5	100 Hz		5.000	4.956	+0.044	1.6
*6	100 Hz		6.000	5.929	+0.071	1.5
*7	100 Hz		7.000	6.919	+0.081	1.5

Certificate No. Q24037354

F3-011-05/12-23

page 3 of 4

เอกสารไม่ควบคุม



@clccalibration



# CALIBRATION LABORATORY Co.,LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230  
Tel. 02-578-0353-4 Fax. 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



# CALIBRATION LABORATORY Co.,LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230  
Tel. 02-578-0353-4 Fax. 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



#### CALIBRATION DATA

##### 3. DISPLACEMENT RESULT

Test point		Mode	STD Reading	DUC Reading	Correction	Uncertainty
(mm)	(frequency)		(mm)	(mm)	(mm)	± (% of rdg.)
0.03	50 Hz	peak	0.030	0.030	0.000	2.5
0.04	50 Hz		0.040	0.040	0.000	2.1
0.05	50 Hz		0.050	0.050	0.000	1.9
0.06	50 Hz		0.060	0.059	+0.001	1.8
0.07	50 Hz		0.070	0.069	+0.001	1.8
0.03	100 Hz	peak	0.030	0.030	0.000	2.5
0.04	100 Hz		0.040	0.040	0.000	2.1
0.05	100 Hz		0.050	0.050	0.000	1.9
0.06	100 Hz		0.060	0.059	+0.001	1.8
0.07	100 Hz		0.070	0.069	+0.001	1.8

Note. The Scope of Accredited ANAB Certificate No. ACDM-2814 Version 012 Page 1,2 of 67

\* means Calibrations marked \* Not ANAB Accredited \* in this Certificate have been included for completeness.

This report is valid for the above stated instrument/s only.

### End of Certificate ###

Certificate No. Q24037354

F3-011-05/12-23

page 4 of 4

เอกสารไม่ควบคุม



@clccalibration

## CERTIFICATE OF CALIBRATION

### FOR

NOMENCLATURE : VIBRATION METER  
MANUFACTURER : INSTANTEL  
MODEL / TYPE : 721A2601/721A3301  
SERIAL NO. : UM11059/UM11059  
CLID. NO. : 252000388  
JOB CONTROL NO. : 240406037352  
CALIBRATION SERVICE : ☒ IN-LABORATORY ☐ ON-SITE

CUSTOMER : UNITED ANALYST AND ENGINEERING CONSULTANT CO., LTD.  
81 SOI UDOMSUK 41, SUKHUMVIT ROAD,  
BANGCHAK, PHRAKHANONG, BANGKOK 10260

DATE OF RECEIVED : 06 April 2024

DATE OF ISSUED : 10 April 2024

The report of calibration shall not be reproduced except in full without approval of the Calibration Laboratory Co., Ltd.

Calibrated By :

Suwit Phuanbusabong  
Calibration Engineer

Approved By :

Authorized Signatory  
10 April 2024

This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to the  
International System of Units (SI)

Certificate No. Q24037352

F3-011-05/12-23

page 1 of 4

เอกสารไม่ควบคุม



@clccalibration



# CALIBRATION LABORATORY CO., LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230  
Tel. 02-578-0353-4 Fax. 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



# CALIBRATION LABORATORY CO., LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230  
Tel. 02-578-0353-4 Fax. 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



## REPORT OF CALIBRATION

### FOR

NOMENCLATURE : VIBRATION METER  
MANUFACTURER : INSTANTEL  
MODEL / TYPE : 721A2601/721A3301  
SERIAL NO. : UM11059/UM11059  
DATE OF CALIBRATION : 08 April 2024

#### ENVIRONMENT CONDITIONS :

Temperature : (23 ± 2) °C Relative Humidity : (55 ± 15) %RH

#### PROCEDURE USED :

This instrument was calibrated under procedure No. CLC-CPEE-08 based on ISO 16063-21 as calibration guideline.  
The calibration was performed by using Digital Multimeter, Universal Counter, Accelerometer and Measuring Amplifier which maintained by the Calibration Laboratory Co., Ltd.

#### REFERENCE STANDARD USED :

- Digital Multimeter, Wavetek Model 1281 S/N. 29320.
- Universal Counter, Hewlett Packard Model 5315A S/N. 2448A13042.
- Accelerometer with Measuring Amplifier, Bruel & Kjaer Model 8305, 2525 S/N. 397018, 2434988.

#### TRACEABILITY :

- The measurements are traceable to International System of Units (SI), through Aeronautical Radio of Thailand Ltd. Certificate No. 05-0316/23, Due Date 21 July 2025.
- The measurements are traceable to International System of Units (SI), through Aeronautical Radio of Thailand Ltd. Certificate No. 07-0159/23, Due Date 04 December 2024.
- The measurements are traceable to International System of Units (SI), through National Institute of Metrology (Thailand) Certificate No. AV-0052-23, Due Date 26 September 2024.

#### UNCERTAINTY :

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor  $k = 2.00$  which for a normal distribution corresponds to a coverage probability of approximately 95 %.  
It has been evaluated according to the "Evaluation of the Uncertainty of Measurement in Calibration (EA-4/02 M:2022)"

Certificate No. Q24037352

F3-011-05/12-23

page 2 of 4

เอกสารไม่ควบคุม



@cdccalibration

## CONDITION OF CALIBRATION ITEM : RECEIVED IN GOOD OPERATIONAL CONDITION

MEASUREMENT RESULTS : (X) without adjustment ( ) adjustment

### CALIBRATION DATA

#### 1. ACCELERATION RESULT

Test point		Mode	STD Reading	DUC Reading	Correction	Uncertainty
( g )	( frequency )		( g )	( g )	( g )	± ( % of rdg. )
0.3	50 Hz	peak	0.300	0.303	-0.003	1.9
0.4	50 Hz		0.400	0.404	-0.004	1.6
0.5	50 Hz		0.500	0.505	-0.005	1.6
0.6	50 Hz		0.600	0.606	-0.006	2.5
0.7	50 Hz		0.700	0.708	-0.008	2.5
0.3	100 Hz	peak	0.300	0.302	-0.002	1.9
0.4	100 Hz		0.400	0.403	-0.003	1.6
0.5	100 Hz		0.500	0.504	-0.004	1.6
0.6	100 Hz		0.600	0.607	-0.007	2.5
0.7	100 Hz		0.700	0.709	-0.009	2.5

#### 2. VELOCITY RESULT

Test point		Mode	STD Reading	DUC Reading	Correction	Uncertainty
( mm/s )	( frequency )		( mm/s )	( mm/s )	( mm/s )	± ( % of rdg. )
3	50 Hz	peak	3.000	3.035	-0.035	1.8
4	50 Hz		4.000	4.041	-0.041	1.8
5	50 Hz		5.000	5.056	-0.056	1.8
6	50 Hz		6.000	6.068	-0.068	1.8
7	50 Hz		7.000	7.071	-0.071	1.8
*3	100 Hz	peak	3.000	3.046	-0.046	1.6
*4	100 Hz		4.000	4.051	-0.051	1.6
*5	100 Hz		5.000	5.063	-0.063	1.6
*6	100 Hz		6.000	6.072	-0.072	1.5
*7	100 Hz		7.000	7.088	-0.088	1.5

Certificate No. Q24037352

F3-011-05/12-23

page 3 of 4

เอกสารไม่ควบคุม



@cdccalibration



# CALIBRATION LABORATORY CO., LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230  
Tel. 02-578-0353-4 Fax. 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



### CALIBRATION DATA

#### 3. DISPLACEMENT RESULT

Test point		Mode	STD Reading	DUC Reading	Correction	Uncertainty
( mm )	( frequency )		( mm )	( mm )	( mm )	± ( % of rdg. )
0.03	50 Hz	peak	0.030	0.030	0.000	2.5
0.04	50 Hz		0.040	0.040	0.000	2.1
0.05	50 Hz		0.050	0.050	0.000	1.9
0.06	50 Hz		0.060	0.060	0.000	1.8
0.07	50 Hz		0.070	0.071	-0.001	1.8
0.03	100 Hz	peak	0.030	0.030	0.000	2.5
0.04	100 Hz		0.040	0.040	0.000	2.1
0.05	100 Hz		0.050	0.050	0.000	1.9
0.06	100 Hz		0.060	0.061	-0.001	1.8
0.07	100 Hz		0.070	0.071	-0.001	1.8

Note. The Scope of Accredited ANAB Certificate No. ACDM-2814 Version 012 Page 1,2 of 67

\* means Calibrations marked \* Not ANAB Accredited \* in this Certificate have been included for completeness.

This report is valid for the above stated instrument/s only.

### End of Certificate ###

Certificate No. Q24037352

F3-011-05/12-23

page 4 of 4

เอกสารไม่ควบคุม



@cdccalibration

INNOVATIVE INSTRUMENT CALIBRATION LAB

INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE

7/139 MOO 13, SOI SUTINAKORN 11 TAMBON BANG KAE0,

AMPHOE BANG PHU SAMUT, PRAKAN PROVINCE 10540 THAILAND

TEL: (66)0-2116-5860-1 FAX: (66)0-2116-7140



Page 1 of 3

### Certificate of Calibration

#### Customer

Name : UNITED ANALYST AND ENGINEERING  
CONSULTANT CO.,LTD.  
Address : 81 Soi Udomsuk 41, Sukhumvit Road, Bangchak,  
Prakanong, Bangkok 10260

Certificate No : 24-ACT-091

Request No : Req-2024-1380

#### Unit Under Calibration Details

Measurement item : Acoustic Calibrator  
Manufacturer : SVANTEK  
Model : SV 36  
Serial Number : 107224  
ID : UAE.EFM.171/2564

Class : 1  
Range : 94 , 114 dB / 1000 Hz  
Instrument Status : Used

#### Calibration Environment and Details

Temperature : ( 23 ± 2 °C )  
Humidity : ( 50 ± 20 %RH )  
Barometric Pressure : ( 1013 ± 10.0 hPa )  
Received Date : 24 June 2024  
Calibration Date : 26 June 2024  
Location of Calibration : LAB 1 Acoustic  
Calibration Procedure : In-house method CP-ACT-02 based on IEC 60942:2017 Electroacoustics - Sound calibrators

Reference Standard	Model	Serial Number	Traceable	Due Calibration
Sound Calibrator	SV 35A	58079	EEL	12 June 2025
THD Multimeter	2015	1047765	NIMT	16 January 2025

Traceability : This certificate provides traceability of measurement to recognized national standard, and to the realization of the international System of Units (SI).

#### Note

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor  $k = 2$ , providing a level of confidence approximately 95 %.

Calibrated By :



Service Calibration Engineer

Approved By :



Calibration Engineer Supervisor


Issue Date : 26 June 2024

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Issuing Laboratory.

เอกสารไม่ควบคุม

PM-708-ACT-02 Rev.03 Issue date 5/6/24





Certificate No : 24-ACT-091

Request No : Req-2024-1380

Calibration Results : Without Adjustment

Sound pressure level

Calibration Range (dB)	Without Adjustment (dB)		Adjustment (dB)		Uncertainty ( ± dB)	Acceptance limit Class 1 ( ± dB)	Result
	Measured	Deviated value	Measured	Deviated value			
94 dB / 1000 Hz	94.02	0.02	-	-	0.14	0.25	Pass
114 dB / 1000 Hz	114.05	0.05	-	-	0.13	0.25	Pass

Frequency of Sound pressure level

Calibration Range (Hz)	Without Adjustment		Adjustment		Uncertainty ( ± %)	Acceptance limit Class 1 ( ± %)	Result
	Measured (Hz)	Deviated	Measured (Hz)	Deviated			
94 dB / 1000 Hz	1000.00	0.00	-	-	0.01	0.70	Pass
114 dB / 1000 Hz	1000.00	0.00	-	-	0.01	0.70	Pass

Total Harmonic Distortion plus Noise of Sound pressure level (THD+N %)

Calibration Range (Hz)	Without Adjustment		Adjustment		Uncertainty ( ± %)	Acceptance limit Class 1 ( ± %)	Result
	Measured (%)	Deviated	Measured (%)	Deviated			
94 dB / 1000 Hz	0.24		-		0.40	2.5	Pass
114 dB / 1000 Hz	0.44		-		0.40	2.5	Pass

Note :

Function	Maximum-permitted Uncertainty of measurement
Sound pressure level	0.15 dB
Frequency	0.20%
Total distortion+noise	0.50%

~ Acceptance limit was IEC60942:2017 Class 1


~ The calibration results exclude the calibrator pressure correction

~ The calibration results exclude the microphone volume correction

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Issuing Authority.

เอกสารไม่ควบคุม

FM-708-ACT-02 Rev.03 Issue date 5/6/24



Certificate No : 24-ACT-091

Request No : Req-2024-1380

Decision Rule for Statements of Conformity


The standard decision rule employed for the statements of conformity to each calibration result will be applied using ILAC-G8:09/2019: Guidelines on the Reporting of Compliance with Specification as following Fig. and statements

Pass = The measurement result plus the expanded uncertainty with a 95% coverage probability were within the limit.

Pass<sup>1</sup> = The measurement result was within the limit. However, a portion of the expanded uncertainty of measurement at 95% exceeds the limit.

Fail<sup>1</sup> = The measurement result was out of the limit. However, a portion of the expanded uncertainty of measurement at 95% is within the limit.

Fail = The measurement result plus the expanded uncertainty with a 95% coverage probability were outside the limit.

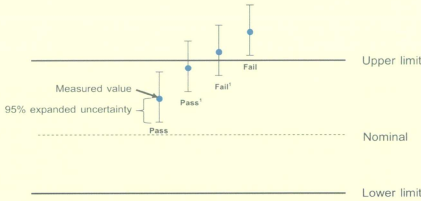

End of Calibration

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Issuing Authority.

เอกสารไม่ควบคุม

FM-708-ACT-02 Rev.03 Issue date 5/6/24



Certificate of Calibration

Customer

Name : UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.

Certificate No : 24-SLM-234

Address : 81 Soi Udomsak 41, Sukhumvit Road, Bangchak, Prakanong, Bangkok

Request No : Req-2024-1453

10260

Unit Under Calibration Details

Measurement item : Sound Level Meter

Microphone Class : 2

Manufacturer : Larson Davis

Microphone Model : 375B02

Model : LX12

Microphone S/N : 011740

Serial Number : 0005286

Preamplifier Model : PRMLX12B

ID : UAE.EFM.102/2562

Preamplifier S/N : 056087

Resolution : 0.1 dB

Instrument Status : Used

Calibration Environment and Details

Temperature : 23 °C ± 2 °C

Humidity : 50 %RH ± 20 %RH

Barometric Pressure : 1013 hPa ± 10 hPa

Received Date : 1 July 2024

Calibrated Date : 10 July 2024

Calibration Procedure : In-house method CP-SLM-01 based on IEC 61672-3 : 2013 Electroacoustics - Sound level meters - Part 3: Periodic tests

Location of Calibration : Lab Acoustic


Reference Standard

Instrument	Brand	Model	SN.	Due calibration	Traceability
Standard Microphone	GRAS	40AN	188273	20 August 2024	GRAS
Multifrequency Calibrator	Quest	Quest-cal	EFA000234	26 July 2024	TSI
Audio Generator	Svante	Svan401	131	8 October 2024	WK Electric

Note


The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor  $k = 2$ , providing a level of confidence approximately 95 %.

Calibrated By :



Service Calibration Engineer

Approved By :




Calibration Engineer Supervisor

Issue Date : 10 July 2024

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Issuing Authority.

เอกสารไม่ควบคุม

FM-708-SLM-01 Rev.04 Issue date 5/6/24



Certificate No : 24-SLM-234

Request No : Req-2024-1453

1. Indication at the calibration check frequency

UUC Setting FAST / A / 37-139	Nominal Level (dB)	Before Adjust		After Adjust		UNCERTAINTY ( ± dB)	Acceptance Limit ( ± dB)	Result
		UUC (dB)	ERR (dB)	UUC (dB)	ERR (dB)			
Calibrator Setting								
1000 Hz 114 dB	113.76	114.4	0.64	113.8	+0.04	0.20	0.30	Pass

Note : Absolute sensitivity was established by the use of Sound Calibrator Brand SVANTEK, Model SV 35A, SN. 58079

2. Self-generated noise, Microphone installed

UUC Setting FAST / 37-139	Measured (dB)	UNCERTAINTY ( ± dB)
A	31.3	0.10

3. Self-generated noise, Microphone replaced by the electrical input signal device

UUC Setting FAST / 37-139	Measured (dB)	UNCERTAINTY ( ± dB)
A	31.1	0.10
C	30.6	0.10
Z	34.9	0.10

4. Acoustic signal test of frequency weightings (Without Windscreen)

UUC Setting FAST / 37-139	Deviation from various Frequency Weighting Responce curve			UNCERTAINTY ( ± dB)	Acceptance Limit ( ± dB)	Result
	STD Setting (dB)	A (dB)	C (dB)			
125 Hz	0.0	0.1	0.1	0.60	1.5	Pass
1000 Hz	0.0	0.0	0.0	0.60	1.0	Pass
4000 Hz	1.2	1.2	1.2	0.60	3.0	Pass
8000 Hz	2.7	2.8	2.9	0.70	5.0	Pass <sup>1</sup>

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Issuing Authority.

เอกสารไม่ควบคุม

FM-708-SLM-01 Rev.04 Issue date 5/6/24

5. Electrical signal test of frequency weightings, Weighting network response with relative to 1 kHz

UUC Setting	Deviation from various Frequency			UNCERTAINTY	Acceptance	Result
FAST / 37-139	Weighting Response curve				Limit	
STD Setting	A (dB)	C (dB)	Z (dB)	(± dB)	(± dB)	
63 Hz	-0.1	0.0	0.0	0.20	2.0	Pass
125 Hz	-0.1	0.0	0.0		1.5	Pass
250 Hz	-0.1	0.0	0.0		1.5	Pass
500 Hz	0.0	0.1	0.0		1.5	Pass
1000 Hz	0.0	0.0	0.0		1.0	Pass
2000 Hz	0.0	0.1	0.0		2.0	Pass
4000 Hz	0.0	0.0	0.0		3.0	Pass
8000 Hz	0.0	0.0	0.0		5.0	Pass
16000 Hz	0.0	-0.1	-0.1		+5, -INF.	Pass

6. Frequency and time weightings at 1kHz

UUC Setting	STD	Measured		UNCERTAINTY	Acceptance Limit	Result
FAST / 37-139	REF	UUC	ERR			
UUC Weighting	(dB)	(dB)	(dB)	(± dB)	(± dB)	
A	114.00	114.0	0.0	0.20	0.20	Pass
C	114.00	114.0	0.0		0.20	Pass
Z	114.00	114.0	0.0		0.20	Pass

UUC Setting	STD	Measured		UNCERTAINTY	Acceptance Limit	Result
37-139 / A	REF	UUC	ERR			
UUC Time Response	(dB)	(dB)	(dB)	(± dB)	(± dB)	
Fast	114.00	114.0	0.0	0.20	0.10	PassI
Slow	114.00	114.0	0.0		0.10	PassI
Leq	114.00	114.0	0.0		0.10	PassI

7. Long Term Stability

UUC Setting	Measured	UNCERTAINTY	Acceptance Limit	Result
FAST / A / 37-139	UUC			
STD Setting	(dB)	(± dB)	(± dB)	
Initial	114.0			
Final	114.0			
Deviated	0.0	0.10	0.30	Pass

8. Level linearity on the reference level range

UUC Setting	Anticipated	Deviation		UNCERTAINTY	Acceptance Limit	Result
FAST / A / 37-139	REF	UUC	ERR			
STD dB	(dB)	(dB)	(dB)	(± dB)	(± dB)	
139.00	139	139.0	0.0	0.30	1.1	Pass
134.00	134	134.0	0.0		1.1	Pass
129.00	129	129.0	0.0		1.1	Pass
124.00	124	124.0	0.0		1.1	Pass
119.00	119	119.0	0.0		1.1	Pass
114.00	114	114.0	0.0		1.1	Pass
109.00	109	109.0	0.0		1.1	Pass
104.00	104	104.0	0.0		1.1	Pass
99.00	99	99.0	0.0		1.1	Pass
94.00	94	94.0	0.0		1.1	Pass
89.00	89	89.0	0.0		1.1	Pass
84.00	84	84.0	0.0		1.1	Pass
79.00	79	79.0	0.0		1.1	Pass
74.00	74	74.0	0.0		1.1	Pass
69.00	69	69.0	0.0		1.1	Pass
64.00	64	64.0	0.0		1.1	Pass
59.00	59	59.0	0.0		1.1	Pass
54.00	54	54.0	0.0		1.1	Pass
49.00	49	49.1	0.1		1.1	Pass
44.00	44	44.2	0.2		1.1	Pass
43.00	43	43.3	0.3		1.1	Pass
42.00	42	42.3	0.3		1.1	Pass
41.00	41	41.4	0.4		1.1	Pass

9. Level linearity including the level range control

UUC Setting	STD	Measured		UNCERTAINTY	Acceptance Limit	Result
FAST / A	REF	UUC	ERR			
UUC Range	(dB)	(dB)	(dB)	(± dB)	(± dB)	
37-139	46.30	46.4	0.1	0.30	1.1	Pass
	114	114.0	0.0		1.1	Pass

10. Tone burst response

UUC Setting	STD	Anticipated	Measured		UNCERTAINTY	Acceptance Limit	Result
A / 37-139	Toneburst	Ref	UUC	ERR			
UUC Time Response	(ms)	(dB)	(dB)	(dB)	(± dB)	(± dB)	
Fast	200	135.0	134.9	-0.1	0.20	1.0	Pass
	2	118.0	117.6	-0.4		+1.0, -2.5	Pass
	0.25	109.0	108.6	-0.4		+1.5, -5.0	Pass
Slow	200	128.6	128.5	-0.1		1.0	Pass
	2	109.0	108.9	-0.1		+1.0, -5.0	Pass
	200	129.0	129.0	0.0		1.0	Pass
SEL	2	109.0	109.0	0.0		+1.0, -2.5	Pass
	0.25	100.0	99.8	-0.2		+1.5, -5.0	Pass

11. Peak C Sound level

UUC Setting	Anticipated	Measured		UNCERTAINTY	Acceptance Limit	Result
FAST / C / 95-142	REF	UUC	ERR			
STD Setting	(dB)	(dB)	(dB)	(± dB)	(± dB)	
Complete cycle	137.4	136.8	-0.60	0.20	3.0	Pass
Positive half cycle	136.4	136.2	-0.20		2.0	Pass
Negative half cycle	136.4	136.2	-0.20		2.0	Pass

12. Overload indication

UUC Setting	Measured	UNCERTAINTY	Acceptance Limit	Result
FAST / A / 37-139	UUC			
STD Setting	(dB)	(± dB)	(± dB)	
Positive one-half cycle	145.5			
Negative one-half cycle	145.4			
Deviated	0.1	0.20	1.5	Pass

13. High Level Stability

UUC Setting	Measured	UNCERTAINTY	Acceptance Limit	Result
FAST / A / 37-139	UUC			
STD Setting	(dB)	(± dB)	(± dB)	
Initial	138.0			
Final	138.0			
Deviated	0.0	0.10	0.30	Pass

Note :

Function	Maximum-permitted Uncertainty of measurement
1. Indication at the calibration check frequency	Not applicable
2. Self-generated noise, Microphone installed	Not applicable
3. Self-generated noise, Microphone replaced by the electrical input signal device	Not applicable
4. Acoustic signal test of frequency weightings at 10 Hz to 4 kHz	0.60 dB
4. Acoustic signal test of frequency weightings at >4 kHz to 10 kHz	0.70 dB
5. Electrical signal test of frequency weightings, Weighting network response with relative to 1 kHz	0.20 dB
6. Frequency and time weightings at 1kHz	0.20 dB
7. Long Term Stability	0.10 dB
8. Level linearity on the reference level range	0.30 dB
9. Level linearity including the level range control	0.30 dB
10. Tone burst response	0.30 dB
11. Peak C Sound level	0.35 dB
12. Overload indication	0.25 dB
13. High Level Stability	0.10 dB

- Acceptance limit and Maximum-permitted Uncertainty was IEC 61672-1:2013



Certificate No : 24-SLM-234  
Request No : Req-2024-1453

#### Decision Rule for Statements of Conformity


The standard decision rule employed for the statements of conformity to each calibration result will be applied using ILAC-G8:09/2019: Guidelines on the Reporting of Compliance with Specification as following Fig. and statements

Pass = The measurement result plus the expanded uncertainty with a 95% coverage probability were within the limit.

Pass<sup>1</sup> = The measurement result was within the limit. However, a portion of the expanded uncertainty of measurement at 95% exceeds the limit.

Fail<sup>1</sup> = The measurement result was out of the limit. However, a portion of the expanded uncertainty of measurement at 95% is within the limit.

Fail = The measurement result plus the expanded uncertainty with a 95% coverage probability were outside the limit.

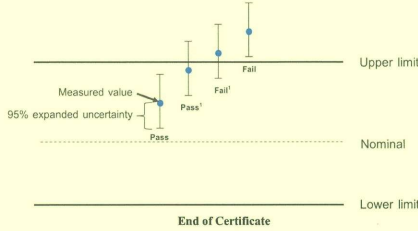

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of

เอกสารไม่ควบคุม

FM-708-SLM-01 Rev.04 Issue date 5/6/24

#### Certificate of Calibration

##### Customer

Name : UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.  
Address : 81 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Prakanong, Bangkok  
10260

Certificate No : 24-SLM-238

Request No : Req-2024-1457

##### Unit Under Calibration Details

Measurement item : Sound Level Meter  
Manufacturer : Larson Davis  
Model : LxT2  
Serial Number : 0005290  
ID : UAE.EFM.106/2562  
Resolution : 0.1 dB  
Microphone Class : 2  
Microphone Model : 375A04  
Microphone S/N : 351857  
Preamplifier Model : PRMLxT2B  
Preamplifier S/N : 056077  
Instrument Status : Used

##### Calibration Environment and Details

Temperature : 23 °C ± 2 °C  
Humidity : 50 %RH ± 20 %RH  
Barometric Pressure : 1013 hPa ± 10 hPa  
Received Date : 2 July 2024  
Calibrated Date : 11 July 2024  
Calibration Procedure : In-house method CP-SLM-01 based on IEC 61672-3 : 2013 Electroacoustics - Sound level meters - Part 3: Periodic tests  
Location of Calibration : Lab Acoustic

##### Reference Standard

Instrument	Brand	Model	SN.	Due calibration	Traceability
Standard Microphone	GRAS	40AN	188273	20 August 2024	GRAS
Multifrequency Calibrator	Quest	Quest-cal	EFA000234	26 July 2024	TSI
Audio Generator	Svantek	Svan401	131	8 October 2024	WK Electric

##### Note

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor  $k = 2$ , providing a level of confidence approximately 95 %.

Calibrated By :



Service Calibration Engineer

Approved By :



Calibration Engineer Supervisor

Issue Date : 11 July 2024

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of

เอกสารไม่ควบคุม

FM-708-SLM-01 Rev.04 Issue date 5/6/24

Certificate No : 24-SLM-238  
Request No : Req-2024-1457

#### 1. Indication at the calibration check frequency

UUC Setting	Nominal	Before Adjust		After Adjust		UNCERTAINTY (± dB)	Acceptance Limit (± dB)	Result
FAST / A / 37-139	Level	UUC	ERR	UUC	ERR			
Calibrator Setting	(dB)	(dB)	(dB)	(dB)	(dB)			
1000 Hz: 114 dB	113.76	114.1	0.34	113.8	+0.04	0.20	0.30	Pass

Note : Absolute sensitivity was established by the use of Sound Calibrator Brand SVANTEK, Model SV 35A, SN. 58079

#### 2. Self-generated noise, Microphone installed

UUC Setting	Measured	UNCERTAINTY
FAST / 37-139	(dB)	(± dB)
A	25.4	0.10

#### 3. Self-generated noise, Microphone replaced by the electrical input signal device

UUC Setting	Measured	UNCERTAINTY
FAST / 37-139	(dB)	(± dB)
A	24.8	0.10
C	24.3	0.10
Z	28.6	0.10

#### 4. Acoustic signal test of frequency weightings (Without Windscreen)

UUC Setting	Deviation from various Frequency Weighting Response curve			UNCERTAINTY (± dB)	Acceptance Limit (± dB)	Result
	A	C	Z			
FAST / 37-139	(dB)	(dB)	(dB)	(± dB)	(± dB)	
125 Hz	0.1	0.2	0.2	0.60	1.5	Pass
1000 Hz	0.0	0.0	0.0	0.60	1.0	Pass
4000 Hz	0.6	0.6	0.6	0.60	3.0	Pass
8000 Hz	0.8	0.8	0.9	0.70	5.0	Pass

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of

เอกสารไม่ควบคุม

FM-708-SLM-01 Rev.04 Issue date 5/6/24

Certificate No : 24-SLM-238  
Request No : Req-2024-1457

#### 5. Electrical signal test of frequency weightings, Weighting network response with relative to 1 kHz

UUC Setting	Deviation from various Frequency Weighting Response curve			UNCERTAINTY (± dB)	Acceptance Limit (± dB)	Result
FAST / 37-139	A	C	Z			
STD Setting	(dB)	(dB)	(dB)	(± dB)	(± dB)	
63 Hz	-0.2	-0.1	-0.1	0.20	2.0	Pass
125 Hz	-0.1	0.0	-0.1		1.5	Pass
250 Hz	-0.1	0.0	-0.1		1.5	Pass
500 Hz	-0.1	0.0	-0.1		1.5	Pass
1000 Hz	0.0	0.0	-0.1		1.0	Pass
2000 Hz	0.0	0.0	0.0		2.0	Pass
4000 Hz	0.0	0.0	0.0		3.0	Pass
8000 Hz	-0.1	-0.1	0.0		5.0	Pass
16000 Hz	-0.1	-0.1	-0.1		+5, -INF.	Pass

#### 6. Frequency and time weightings at 1kHz

UUC Setting	STD	Measured		UNCERTAINTY (± dB)	Acceptance Limit (± dB)	Result
FAST / 37-139	REF	UUC	ERR			
UUC Weighting	(dB)	(dB)	(dB)	(± dB)	(± dB)	
A	114.00	114.0	0.0	0.20	0.20	Pass
C	114.00	114.0	0.0		0.20	Pass
Z	114.00	114.0	0.0		0.20	Pass

UUC Setting	STD	Measured		UNCERTAINTY (± dB)	Acceptance Limit (± dB)	Result
37-139 / A	REF	UUC	ERR			
UUC Time Response	(dB)	(dB)	(dB)	(± dB)	(± dB)	
Fast	114.00	114.0	0.0	0.20	0.10	Pass
Slow	114.00	114.0	0.0		0.10	Pass
Leq	114.00	114.0	0.0		0.10	Pass

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of

เอกสารไม่ควบคุม

FM-708-SLM-01 Rev.04 Issue date 5/6/24



Certificate No : 24-SLM-238  
Request No : Req-2024-1457

7. Long Term Stability

UUC Setting	Measured	UNCERTAINTY (± dB)	Acceptance	Result
FAST / A / 37-139	UUC		Limit	
STD Setting	(dB)			
Initial	114.0			
Final	114.0			
Deviated	0.0	0.10	0.30	Pass

8. Level linearity on the reference level range

UUC Setting	Anticipated	Deviation		UNCERTAINTY	Acceptance	Result
FAST / A / 37-139	REF	UUC	ERR		Limit	
STD dB	(dB)	(dB)	(dB)	(± dB)	(± dB)	
137.00	137	137.0	0.0	0.30	1.1	Pass
134.00	134	134.0	0.0		1.1	Pass
129.00	129	129.0	0.0		1.1	Pass
124.00	124	124.0	0.0		1.1	Pass
119.00	119	119.0	0.0		1.1	Pass
114.00	114	114.0	0.0		1.1	Pass
109.00	109	109.0	0.0		1.1	Pass
104.00	104	104.0	0.0		1.1	Pass
99.00	99	99.0	0.0		1.1	Pass
94.00	94	93.9	-0.1		1.1	Pass
89.00	89	88.9	-0.1		1.1	Pass
84.00	84	83.9	-0.1		1.1	Pass
79.00	79	78.9	-0.1		1.1	Pass
74.00	74	73.9	-0.1		1.1	Pass
69.00	69	68.9	-0.1		1.1	Pass
64.00	64	63.9	-0.1		1.1	Pass
59.00	59	58.9	-0.1		1.1	Pass
54.00	54	53.9	-0.1		1.1	Pass
49.00	49	48.9	-0.1		1.1	Pass
44.00	44	44.0	0.0		1.1	Pass
39.00	39	39.1	0.1		1.1	Pass
38.00	38	38.2	0.2		1.1	Pass
37.00	37	37.2	0.2		1.1	Pass
36.00	36	36.3	0.3		1.1	Pass
35.00	35	35.4	0.4		1.1	Pass

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the client.  
FM-708-SLM-01 Rev.04 Issue date 5/6/24



Certificate No : 24-SLM-238  
Request No : Req-2024-1457

9. Level linearity including the level range control

UUC Setting	STD	Measured		UNCERTAINTY ( ± dB)	Acceptance	Result
FAST / A		REF	UUC		ERR	
UUC Range	(dB)	(dB)	(dB)		( ± dB)	
37-139	40.10	40.2	0.1	0.30	1.1	Pass
	114	114.0	0.0		1.1	Pass

10. Tone burst response

UUC Setting	STD	Anticipated	Measured		UNCERTAINTY	Acceptance	Result
A / 37-139	Toneburst	Ref	UUC	ERR			
UUC Time Response	(ms)	(dB)	(dB)	(dB)	( ± dB)	Limit ( ± dB)	
Fast	200	135.0	135.0	0.0	0.20	1.0	Pass
	2	118.0	117.9	-0.1		+1.0, -2.5	Pass
	0.25	109.0	108.6	-0.4		+1.5, -5.0	Pass
Slow	200	128.6	128.5	-0.1		1.0	Pass
	2	109.0	108.9	-0.1		+1.0, -5.0	Pass
SEL	200	129.0	129.0	0.0		1.0	Pass
	2	109.0	109.0	0.0		+1.0, -2.5	Pass
	0.25	100.0	99.8	-0.2		+1.5, -5.0	Pass

11. Peak C Sound level

UUC Setting	Anticipated	Measured		UNCERTAINTY  ( ± dB)	Acceptance	Result
FAST / C / 95-142	REF	UUC	ERR		Limit	
STD Setting	(dB)	(dB)	(dB)		( ± dB)	
Complete cycle	137.4	136.6	-0.80	0.20	3.0	Pass
Positive half cycle	136.4	136.2	-0.20		2.0	Pass
Negative half cycle	136.4	136.2	-0.20		2.0	Pass

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the client.  
FM-708-SLM-01 Rev.04 Issue date 5/6/24



Certificate No : 24-SLM-238  
Request No : Req-2024-1457

12. Overload indication

UUC Setting	Measured	UNCERTAINTY (± dB)	Acceptance	Result
FAST / A / 37-139	UUC		Limit	
STD Setting	(dB)		(± dB)	
Positive one-half cycle	138.8			
Negative one-half cycle	138.7			
Deviated	0.1	0.20	1.5	Pass

13. High Level Stability

UUC Setting	Measured	UNCERTAINTY  ( ± dB)	Acceptance	Result
FAST / A / 37-139	UUC		Limit	
STD Setting	(dB)		( ± dB)	
Initial	138.0			
Final	138.0			
Deviated	0.0	0.10	0.30	Pass

Note :

Function	Maximum-permitted Uncertainty of measurement
1. Indication at the calibration check frequency	Not applicable
2. Self-generated noise, Microphone installed	Not applicable
3. Self-generated noise, Microphone replaced by the electrical input signal device	Not applicable
4. Acoustic signal test of frequency weightings at 10 Hz to 4 kHz	0.60 dB
4. Acoustic signal test of frequency weightings at >4 kHz to 10 kHz	0.70 dB
5. Electrical signal test of frequency weightings, Weighting network response with relative to 1 kHz	0.20 dB
6. Frequency and time weightings at 1kHz	0.20 dB
7. Long Term Stability	0.10 dB
8. Level linearity on the reference level range	0.30 dB
9. Level linearity including the level range control	0.30 dB
10. Tone burst response	0.30 dB
11. Peak C Sound level	0.35 dB
12. Overload indication	0.25 dB
13. High Level Stability	0.10 dB

- Acceptance limit and Maximum-permitted Uncertainty was IEC 61672-1:2013

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the client.  
FM-708-SLM-01 Rev.04 Issue date 5/6/24



Certificate No : 24-SLM-238  
Request No : Req-2024-1457

Decision Rule for Statements of Conformity


The standard decision rule employed for the statements of conformity to each calibration result will be applied using ILAC-G8:09/2019: Guidelines on the Reporting of Compliance with Specification as following Fig. and statements

Pass = The measurement result plus the expanded uncertainty with a 95% coverage probability were within the limit.

Pass<sup>1</sup> = The measurement result was within the limit. However, a portion of the expanded uncertainty of measurement at 95% exceeds the limit.

Fail<sup>2</sup> = The measurement result was out of the limit. However, a portion of the expanded uncertainty of measurement at 95% is within the limit.

Fail = The measurement result plus the expanded uncertainty with a 95% coverage probability were outside the limit.

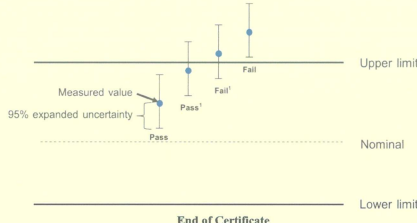

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the client.  
FM-708-SLM-01 Rev.04 Issue date 5/6/24







Certificate No : 24-SLM-231  
Request No : Req-2024-1450

9. Level linearity including the level range control

U/C Setting	STD	Measured		UNCERTAINTY  ( ± dB)	Acceptance Limit	Result
FAST / A	REF	U/C (dB)	ERR (dB)		( ± dB)	
U/C Range	(dB)	(dB)	(dB)			
37-139	44.80	44.9	0.1	0.30	1.1	Pass
	114	114.0	0.0		1.1	Pass

10. Tone burst response

UUC Setting	STD	Anticipated	Measured		UNCERTAINTY  ( ± dB)	Acceptance	Result
A / 37-139	Toneburst	Ref	UUC	ERR		Limit ( ± dB)	
UUC Time Response	(ms)	(dB)	(dB)	(dB)			
Fast	200	135.0	135.0	0.0	0.20	1.0	Pass
	2	118.0	117.9	-0.1		+1.0, -2.5	Pass
	0.25	109.0	108.6	-0.4		+1.5, -5.0	Pass
Slow	200	128.6	128.5	-0.1		1.0	Pass
	2	109.0	108.9	-0.1		+1.0, -5.0	Pass
	200	129.0	129.0	0.0		1.0	Pass
SEL	2	109.0	109.1	+0.1		+1.0, -2.5	Pass
	0.25	100.0	99.8	-0.2		+1.5, -5.0	Pass

11. Peak C Sound level

UUC Setting	Anticipated	Measured		UNCERTAINTY ( ± dB)	Acceptance	Result
FAST / C / 95-142		REF	UUC		ERR	
STD Setting	(dB)	(dB)	(dB)	0.20	3.0	Pass
Complete cycle	137.4	136.7	-0.70		2.0	Pass
Positive half cycle	136.4	136.2	-0.20		2.0	Pass
Negative half cycle	136.4	136.2	-0.20		2.0	Pass

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of **เอกสารไม่ควบคุม**  
FM-708-SLM-01 Rev.04 Issue date 5/6/24

Certificate No : 24-SLM-231  
Request No : Req-2024-1450

12. Overload indication

UUC Setting	Measured	UNCERTAINTY ( ± dB)	Acceptance	Result
FAST / A / 37-139	UUC		Limit	
STD Setting	(dB)		( ± dB)	
Positive one-half cycle	143.7			
Negative one-half cycle	143.8			
Deviated	-0.1	0.20	1.5	Pass

13. High Level Stability

UUC Setting	Measured	UNCERTAINTY  ( ± dB)	Acceptance	Result
FAST / A / 37-139	UUC		Limit	
STD Setting	(dB)		( ± dB)	
Initial	138.0			
Final	138.0			
Deviated	0.0	0.10	0.30	Pass

Note :

Function	Maximum-permitted Uncertainty of measurement
1. Indication at the calibration check frequency	Not applicable
2. Self-generated noise, Microphone installed	Not applicable
3. Self-generated noise, Microphone replaced by the electrical input signal device	Not applicable
4. Acoustic signal test of frequency weightings at 10 Hz to 4 kHz	0.60 dB
4. Acoustic signal test of frequency weightings at >4 kHz to 10 kHz	0.70 dB
5. Electrical signal test of frequency weightings, Weighting network response with relative to 1 kHz	0.20 dB
6. Frequency and time weightings at 1kHz	0.20 dB
7. Long Term Stability	0.10 dB
8. Level linearity on the reference level range	0.30 dB
9. Level linearity including the level range control	0.30 dB
10. Tone burst response	0.30 dB
11. Peak C Sound level	0.35 dB
12. Overload indication	0.25 dB
13. High Level Stability	0.10 dB

\* Acceptance limit and Maximum-permitted Uncertainty was IEC 61672-1:2013

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of **เอกสารไม่ควบคุม**  
FM-708-SLM-01 Rev.04 Issue date 5/6/24

Certificate No : 24-SLM-231  
Request No : Req-2024-1450

Decision Rule for Statements of Conformity


The standard decision rule employed for the statements of conformity to each calibration result will be applied using ILAC-G8:09/2019: Guidelines on the Reporting of Compliance with Specification as following Fig. and statements

Pass = The measurement result plus the expanded uncertainty with a 95% coverage probability were within the limit.

Pass<sup>1</sup> = The measurement result was within the limit. However, a portion of the expanded uncertainty of measurement at 95% exceeds the limit.

Fail<sup>1</sup> = The measurement result was out of the limit. However, a portion of the expanded uncertainty of measurement at 95% is within the limit.

Fail = The measurement result plus the expanded uncertainty with a 95% coverage probability were outside the limit.

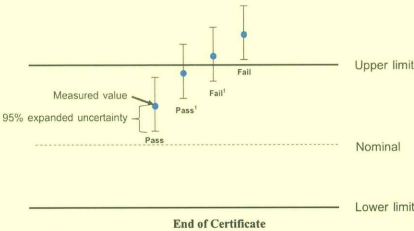

End of Certificate

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of **เอกสารไม่ควบคุม**  
FM-708-SLM-01 Rev.04 Issue date 5/6/24

Certificate of Calibration

Customer

Name : UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.  
Address : 81 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Prakanong, Bangkok 10260

Certificate No : 24-SLM-240  
Request No : Req-2024-1459

Unit Under Calibration Details

Measurement item : Sound Level Meter  
Manufacturer : Larson Davis  
Model : LxT2  
Serial Number : 0005299  
ID : UAE.EFM.114/2562  
Resolution : 0.1 dB

Microphone Class : 2  
Microphone Model : 375A04  
Microphone S/N : 323471  
Preamplifier Model : PRMLXT2C  
Preamplifier S/N : 071493  
Instrument Status : Used

Calibration Environment and Details

Temperature : 23 °C ± 2 °C  
Humidity : 50 %RH ± 20 %RH  
Barometric Pressure : 1013 hPa ± 10 hPa  
Received Date : 2 July 2024  
Calibrated Date : 11 July 2024  
Calibration Procedure : In-house method CP-SLM-01 based on IEC 61672-3 : 2013 Electroacoustics - Sound level meters - Part 3: Periodic tests  
Location of Calibration : Lab Acoustic


Reference Standard

Instrument	Brand	Model	SN.	Due calibration	Traceability
Standard Microphone	GRAS	40AN	188273	20 August 2024	GRAS
Multifrequency Calibrator	Quest	Quest-cal	EFA000234	26 July 2024	TSI
Audio Generator	Svante	Svan401	131	8 October 2024	WK Electric

Note

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor  $k = 2$ , providing a level of confidence approximately 95 %.

Calibrated By :   
Service Calibration Engineer

Approved By :   
Calibration Engineer Supervisor  
Issue Date : 11 July 2024

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of **เอกสารไม่ควบคุม**  
FM-708-SLM-01 Rev.04 Issue date 5/6/24

Certificate No : 24-SLM-240  
Request No : Req-2024-1459

1. Indication at the calibration check frequency

UUC Setting	Nominal	Before Adjust		After Adjust		UNCERTAINTY (± dB)	Acceptance Limit (± dB)	Result
FAST / A / 37-139	Level	UUC (dB)	ERR (dB)	UUC (dB)	ERR (dB)			
Calibrator Setting	(dB)							
1000 Hz 114 dB	113.76	115.3	1.54	113.8	+0.04	0.20	0.30	Pass

Note : Absolute sensitivity was established by the use of Sound Calibrator Brand SVANTEK, Model SV 35A, SN. 58079

2. Self-generated noise, Microphone installed

UUC Setting	Measured (dB)	UNCERTAINTY (± dB)
FAST / 37-139		
UUC Weighting		
A	27.1	0.10

3. Self-generated noise, Microphone replaced by the electrical input signal device

UUC Setting	Measured (dB)	UNCERTAINTY (± dB)
FAST / 37-139		
UUC Weighting		
A	26.6	0.10
C	26.2	0.10
Z	30.6	0.10

4. Acoustic signal test of frequency weightings (Without Windscreen)

UUC Setting	Deviation from various Frequency Weighting Response curve			UNCERTAINTY (± dB)	Acceptance Limit (± dB)	Result
	A	C	Z			
FAST / 37-139	(dB)	(dB)	(dB)			
STD Setting						
125 Hz	0.0	0.2	0.1	0.60	1.5	Pass
1000 Hz	0.0	0.0	0.0	0.60	1.0	Pass
4000 Hz	0.2	0.3	0.4	0.60	3.0	Pass
8000 Hz	-0.5	-0.4	-0.2	0.70	5.0	Pass

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the client.  
FM-708-SLM-01 Rev.04 Issu date 5/6/24

เอกสารไม่ควบคุม

Certificate No : 24-SLM-240  
Request No : Req-2024-1459

5. Electrical signal test of frequency weightings, Weighting network response with relative to 1 kHz

UUC Setting	Deviation from various Frequency Weighting Response curve			UNCERTAINTY (± dB)	Acceptance Limit (± dB)	Result
FAST / 37-139	A (dB)	C (dB)	Z (dB)			
STD Setting						
63 Hz	-0.2	0.0	0.0	0.20	2.0	Pass
125 Hz	-0.1	0.0	0.0		1.5	Pass
250 Hz	-0.1	0.0	0.0		1.5	Pass
500 Hz	-0.1	0.0	0.0		1.5	Pass
1000 Hz	0.0	0.0	0.0		1.0	Pass
2000 Hz	0.0	0.0	0.0		2.0	Pass
4000 Hz	0.0	0.0	0.0		3.0	Pass
8000 Hz	0.0	0.0	0.0		5.0	Pass
16000 Hz	-0.1	-0.1	-0.1		+5, -INF.	Pass

6. Frequency and time weightings at 1kHz

UUC Setting	STD	Measured		UNCERTAINTY (± dB)	Acceptance Limit (± dB)	Result
FAST / 37-139	REF	UUC (dB)	ERR (dB)			
UUC Weighting						
A	114.00	114.0	0.0	0.20	0.20	Pass
C	114.00	114.0	0.0		0.20	Pass
Z	114.00	114.0	0.0		0.20	Pass

UUC Setting	STD	Measured		UNCERTAINTY (± dB)	Acceptance Limit (± dB)	Result
37-139 / A	REF	UUC (dB)	ERR (dB)			
UUC Time Response						
Fast	114.00	114.0	0.0	0.20	0.10	Pass
Slow	114.00	114.0	0.0		0.10	Pass
Leq	114.00	114.0	0.0		0.10	Pass

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the client.  
FM-708-SLM-01 Rev.04 Issu date 5/6/24

เอกสารไม่ควบคุม

Certificate No : 24-SLM-240  
Request No : Req-2024-1459

7. Long Term Stability

UUC Setting	Measured	UNCERTAINTY (± dB)	Acceptance Limit (± dB)	Result
FAST / A / 37-139	UUC			
STD Setting	(dB)			
Initial	114.0			
Final	114.0			
Deviated	0.0			
		0.10	0.30	Pass

8. Level linearity on the reference level range

UUC Setting	Anticipated	Deviation		UNCERTAINTY (± dB)	Acceptance Limit (± dB)	Result
FAST / A / 37-139	REF	UUC (dB)	ERR (dB)			
STD dB	(dB)					
139.00	139	139.0	0.0	0.30	1.1	Pass
134.00	134	134.0	0.0		1.1	Pass
129.00	129	129.0	0.0		1.1	Pass
124.00	124	124.0	0.0		1.1	Pass
119.00	119	119.0	0.0		1.1	Pass
114.00	114	114.0	0.0		1.1	Pass
109.00	109	109.0	0.0		1.1	Pass
104.00	104	104.0	0.0		1.1	Pass
99.00	99	99.0	0.0		1.1	Pass
94.00	94	94.0	0.0		1.1	Pass
89.00	89	89.0	0.0		1.1	Pass
84.00	84	84.0	0.0		1.1	Pass
79.00	79	79.0	0.0		1.1	Pass
74.00	74	74.0	0.0		1.1	Pass
69.00	69	69.0	0.0		1.1	Pass
64.00	64	64.0	0.0		1.1	Pass
59.00	59	59.0	0.0		1.1	Pass
54.00	54	54.0	0.0		1.1	Pass
49.00	49	49.0	0.0		1.1	Pass
44.00	44	44.0	0.0		1.1	Pass
39.00	39	39.2	0.2		1.1	Pass
38.00	38	38.3	0.3		1.1	Pass
37.00	37	37.4	0.4		1.1	Pass
36.00	36	36.5	0.5		1.1	Pass

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the client.  
FM-708-SLM-01 Rev.04 Issu date 5/6/24

เอกสารไม่ควบคุม

Certificate No : 24-SLM-240  
Request No : Req-2024-1459

9. Level linearity including the level range control

UUC Setting	STD	Measured		UNCERTAINTY (± dB)	Acceptance Limit (± dB)	Result
FAST / A	REF	UUC (dB)	ERR (dB)			
UUC Range						
37-139	41.90	42.1	0.2	0.30	1.1	Pass
	114	114.0	0.0		1.1	Pass

10. Tone burst response

UUC Setting	STD	Anticipated	Measured		UNCERTAINTY (± dB)	Acceptance Limit (± dB)	Result
A / 37-139	Toneburst	Ref	UUC (dB)	ERR (dB)			
UUC Time Response	(ms)						
Fast	200	135.0	134.9	-0.1	0.20	1.0	Pass
	2	118.0	117.9	-0.1		+1.0, -2.5	Pass
	0.25	109.0	108.8	-0.2		+1.5, -5.0	Pass
Slow	200	128.6	128.5	-0.1		1.0	Pass
	2	109.0	108.9	-0.1		+1.0, -5.0	Pass
	200	129.0	129.0	0.0		1.0	Pass
SEL	2	109.0	109.1	+0.1		+1.0, -2.5	Pass
	0.25	100.0	100.0	0.0		+1.5, -5.0	Pass

11. Peak C Sound level

UUC Setting	Anticipated	Measured		UNCERTAINTY (± dB)	Acceptance Limit (± dB)	Result
FAST / C / 95-142	REF	UUC (dB)	ERR (dB)			
STD Setting	(dB)					
Complete cycle	137.4	136.6	-0.80	0.20	3.0	Pass
Positive half cycle	136.4	136.2	-0.20		2.0	Pass
Negative half cycle	136.4	136.2	-0.20		2.0	Pass

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the client.  
FM-708-SLM-01 Rev.04 Issu date 5/6/24

เอกสารไม่ควบคุม

Certificate No : 24-SLM-240  
Request No : Req-2024-1459

Page : 6/7

12. Overload indication

UUC Setting	Measured	UNCERTAINTY ( ± dB)	Acceptance	Result
FAST / A / 37-139	UUC		Limit	
STD Setting	(dB)		( ± dB)	
Positive one-half cycle	140.6			
Negative one-half cycle	140.7			
Deviated	-0.1	0.20	1.5	Pass

13. High Level Stability

UUC Setting	Measured	UNCERTAINTY ( ± dB)	Acceptance	Result
FAST / A / 37-139	UUC		Limit	
STD Setting	(dB)		( ± dB)	
Initial	138.0			
Final	138.0			
Deviated	0.0	0.10	0.30	Pass

Note :

Function	Maximum-permitted Uncertainty of measurement
1. Indication at the calibration check frequency	Not applicable
2. Self-generated noise, Microphone installed	Not applicable
3. Self-generated noise, Microphone replaced by the electrical input signal device	Not applicable
4. Acoustic signal test of frequency weightings at 10 Hz to 4 kHz	0.60 dB
4. Acoustic signal test of frequency weightings at >4 kHz to 10 kHz	0.70 dB
5. Electrical signal test of frequency weightings, Weighting network response with relative to 1 kHz	0.20 dB
6. Frequency and time weightings at 1kHz	0.20 dB
7. Long Term Stability	0.10 dB
8. Level linearity on the reference level range	0.30 dB
9. Level linearity including the level range control	0.30 dB
10. Tone burst response	0.30 dB
11. Peak C Sound level	0.35 dB
12. Overload indication	0.25 dB
13. High Level Stability	0.10 dB

- Acceptance limit and Maximum-permitted Uncertainty was IEC 61672-1:2013

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the

เอกสารไม่ควบคุม

FM-708-SLM-01 Rev.04 Issue date 5/6/24

Certificate No : 24-SLM-240  
Request No : Req-2024-1459

Page : 7/7

Decision Rule for Statements of Conformity


The standard decision rule employed for the statements of conformity to each calibration result will be applied using ILAC-G8.09:2019; Guidelines on the Reporting of Compliance with Specification as following Fig. and statements

Pass = The measurement result plus the expanded uncertainty with a 95% coverage probability were within the limit.

Pass<sup>1</sup> = The measurement result was within the limit. However, a portion of the expanded uncertainty of measurement at 95% exceeds the limit.

Fail<sup>2</sup> = The measurement result was out of the limit. However, a portion of the expanded uncertainty of measurement at 95% is within the limit.

Fail = The measurement result plus the expanded uncertainty with a 95% coverage probability were outside the limit.

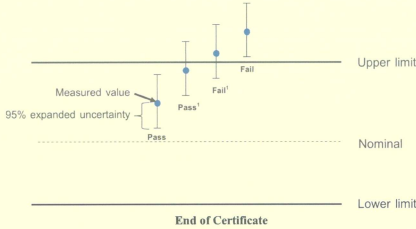

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the

เอกสารไม่ควบคุม

FM-708-SLM-01 Rev.04 Issue date 5/6/24