

ภาคผนวก ค-2

เอกสารสอบเทียบเครื่องมือตรวจวัด



Certificate of Calibration

Calibration Certification Information

Cal. Date: February 9, 2024 Rootsmeter S/N: 438320 Ta: 295 °K
 Operator: Jim Tisch Pa: 749.0 mm Hg
 Calibration Model #: TE-5025A Calibrator S/N: 5411

Run	Vol. Init (m3)	Vol. Final (m3)	ΔVol. (m3)	ΔTime (min)	ΔP (mm Hg)	ΔH (in H2O)
1	1	2	1	1.3950	3.2	2.00
2	3	4	1	0.9840	6.4	4.00
3	5	6	1	0.8790	7.9	5.00
4	7	8	1	0.8430	8.8	5.50
5	9	10	1	0.6940	12.7	8.00

Data Tabulation

Vstd (m3)	Qstd (x-axis)	$\sqrt{\Delta H \left(\frac{Pa}{Pstd} \right) \left(\frac{Tstd}{Ta} \right)}$ (y-axis)	Va	Qa (x-axis)	$\sqrt{\Delta H \left(\frac{Ta}{Pa} \right)}$ (y-axis)
0.9914	0.7106	1.4111	0.9957	0.7138	0.8875
0.9871	1.0032	1.9956	0.9915	1.0076	1.2551
0.9851	1.1207	2.2312	0.9895	1.1257	1.4033
0.9839	1.1672	2.3401	0.9883	1.1723	1.4718
0.9787	1.4103	2.8222	0.9830	1.4165	1.7750
QSTD	m=	2.02024	QA	m=	1.26504
	b=	-0.02667		b=	-0.01677
	r=	0.99993		r=	0.99993

Calculations

Vstd=	$\Delta Vol \left(\frac{Pa - \Delta P}{Pstd} \right) \left(\frac{Tstd}{Ta} \right)$	Va=	$\Delta Vol \left(\frac{Pa - \Delta P}{Pa} \right)$
Qstd=	Vstd/ΔTime	Qa=	Va/ΔTime
For subsequent flow rate calculations:			
Qstd= $1/m \left(\left(\sqrt{\Delta H \left(\frac{Pa}{Pstd} \right) \left(\frac{Tstd}{Ta} \right)} \right) - b \right)$		Qa= $1/m \left(\left(\sqrt{\Delta H \left(\frac{Ta}{Pa} \right)} \right) - b \right)$	

Standard Conditions

Tstd:	298.15 °K
Pstd:	760 mm Hg
Key	
ΔH: calibrator manometer reading (in H2O)	
ΔP: rootsmeter manometer reading (mm Hg)	
Ta: actual absolute temperature (°K)	
Pa: actual barometric pressure (mm Hg)	
b: intercept	
m: slope	

RECALIBRATION

US EPA recommends annual recalibration per 1998 40 Code of Federal Regulations Part 50 to 51, Appendix B to Part 50, Reference Method for the Determination of Suspended Particulate Matter in the Atmosphere, 9.2.17, page 30



CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhprachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech.cal@yahoo.com, calibratech.cal@hotmail.com



Certificate of Calibration

Certificate No. : 67-200034-1

Page : 1 of 2

Submitted by : Envilab Co.,Ltd.
540, 540/1 Soi Bangkhae 7, Bangkhae, Bangkok 10160

Equipment : Electronic Balance
Manufacturer : Sartorius Model : SECURA224-1S
Serial No. : 0034803270 ID No. : ELABBALANCEN04
Capacity : 220 g Resolution : 0.0001 g

Environment : On site calibration was carried out at the Balance Room, Envilab Co., Ltd.
Ambient Temperature : (22.8 to 23.6) °C
Relative Humidity : (44.6 to 45.3) %
Air Pressure : 1014.0 mbar

Date of Received : 01 February 2024

Date of Calibration : 01 February 2024

Date of Issue : 06 February 2024

Calibrated by : Akaradath Thippichai

Calibration Method : In-house method CAL-M2001 based on UKAS Publication ref : LAB 14
Edition 7 - November 2022

Reference Standard Instruments : This certification is traceable to the International System of Units

Standard Weights

<u>ID No.</u>	<u>Cert. No.</u>	<u>Due Date</u>	<u>Traceability</u>
E261-E2624	C02232088	08 Nov 2024	National Institute of Metrology (Thailand), (NIMT)

Approved by :

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhprachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech.cal@yahoo.com, calibratech.cal@hotmail.com

Certificate of Calibration

Certificate No. : 67-200034-1

Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Departure of indication from nominal value


Nominal Value (g)	Correction (g)	Uncertainty \pm (g)
0.01	0.0001	0.00012
0.1	0.0001	0.00012
1	0.0000	0.00013
2	0.0001	0.00013
5	0.0000	0.00013
10	0.0000	0.00013
20	-0.0001	0.00014
50	-0.0001	0.00015
100	-0.0001	0.00020
200	-0.0001	0.00038

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2.06$, providing a level of confidence of approximately 95%

Eccentric error

Load test : 50 g
A B C D E
-0.0001 -0.0001 -0.0001 0.0001 0.0000 g



Repeatability

Load test : 200 g
Stdev. : 0.00005 g

- o0o -



CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhaphrasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech.cal@yahoo.com, calibratech.cal@hotmail.com



NSC-TISI-TIS17025
CALIBRATION 0030

Certificate of Calibration

Certificate No. : 67-410025-1

Page : 1 of 2

Submitted by : Envilab Co., Ltd.
540, 540/1 Soi Bangkhac 7, Bangkhac, Bangkok 10160

Equipment : Digital Thermo-Hygrometer

Manufacturer : Jedto

Model : HTC-1

Range Temperature : N/A °C

Resolution : 0.1 °C

Range Humidity : N/A %R.H.

Resolution : 1 %R.H.

Serial No. : PONPE5852094

ID No. : ELABTMHTC10003

Environment : Ambient Temperature : $(23 \pm 2) ^\circ\text{C}$
Relative Humidity : $(50 \pm 15) \%$

Date of Received : 20 February 2024

Date of Calibration : 22 February 2024

Date of Issue : 22 February 2024

Calibrated by : Chortip Samchusri

Calibration Method : This instrument was calibrated by In-house method comparison technique CAL-M4013 by compared with standard probe sensor humidity/temperature into humidity/temperature chamber.

Reference Standard Instruments : This certification is traceable to the International System of Units

Digital Indicator with Standard Probe Temp&Hum


ID No.	Cert. No.	Due Date	Traceability
400034 & 400035	SG-H-00020/67	05 Jul 2024	Success Gateway Co., Ltd., Accredited by TISI Calibration No.0268

Approved by :



The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhprachasam 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech.cal@yahoo.com, calibratech.cal@hotmail.com

Certificate of Calibration

Certificate No. : 67-410025-1

Page : 2 of 2

UUC Condition As-Received : Good

Result of Calibration : Without Adjustment

Function : Temperature measurement

Reference Humidity @ 50 %R.H.

Standard Temperature (°C)	UUC Reading (°C)	Correction (°C)	Uncertainty (± °C)
24.98	25.0	0.0	0.46

Result of Calibration : Without Adjustment

Function : Humidity measurement

Reference Temperature @ 25 °C

Standard Humidity (%R.H.)	UUC Reading (%R.H.)	Correction (%R.H.)	Uncertainty (± %R.H.)
50.03	50	0	2.2

Remark

UUC : Unit Under Calibration

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

- o0o -



รับรองสำเนา
ถูกต้อง
www.calibratech.co.th



THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804,0-2399-0469

Calibration Certificate

Issued by : Calibration & Test Section : Meteorological Instruments Bureau

Date of Issue 6 April, 2024

Certification No. 172/24

Page : 1 of 6

Object : เครื่องมือตรวจวัดอุตุนิยมวิทยา

Manufacturer : NovaLynx

Type : Data Logger 110-WS-25DL-D

Serial No. : EWSNV110WS2503

Customer : ENVILAB Co.,Ltd.
540, 540/1 Soi Bangkhae 7, Bangkhae, Bangkhae,
Bangkok 10160,Thailand.

Calibration Condition : Temperature 25.1 °C Barometric Pressure 1009.2 hPa

NATIONAL STANDARD WIND TUNNEL : Wind Aloft Plotting Board

: Micromanometer Theodor Friedrichs FC014 Serial No. 9310119 : HOOK GAGE NO 1425

N.I.S.T. Test Reference Number 731/241460 : Standard Velocity at 20 - 30 m/sec

: Ultrasonic Anemometer Model DA-650-3TV (sensor TR-90AH)
Serial Number 110730029 (sensor 120629586)

JAPAN QUALITY ASSURANCE ORGANIZATION : Standard Velocity at 0 - 20 m/sec

STANDARD THERMOMETER : Theodor Friedrich : Dry No.8390/94 Wet No. 8389/94


: Thermoschneider No.9188 : testo, testo 645 Serial No. 02848057

STANDARD BAROMETER : Digital Barometer Vaisala Type PTB220 No. V1220046

Calibrated by : 
Mr. Watcharapong
Mechanical Engineer

(Authorised Signatory)
for the Chief

Sub-Standard



Envilab Co.,Ltd.

รับรองสำเนาถูกต้อง
ผู้จัดการฝ่ายควบคุมคุณภาพ



THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804,0-2399-0469

The Result of Calibration

Sensor model

EWSNV110WS2503

Certification No. 172/24

6 April, 2024

Page : 2 of 6

Standard Ultrasonic Anemometer	HOOK GAGE NO. 1425			TESTED ANEMOMETER	
	Pressure	Vacumm	Velocity	Velocity	Correction
	inches H2O	inches H2O	m/sec	m/sec	m/sec
1.00	-	-	-	0.3	0.70
3.02	-	-	-	2.4	0.62
5.00	-	-	-	4.9	0.10
7.04	-	-	-	6.9	0.14
9.02	-	-	-	8.8	0.22
11.01	-	-	-	10.9	0.11
13.01	-	-	-	12.8	0.21
15.01	-	-	-	15.1	-0.09
17.02	-	-	-	16.8	0.22
20.02	-	-	-	20.1	-0.08

Wind Aloft Plotting Board.	
US.DEPARTMENT OF COMMERCE WEATHER BUREAU	
WIND DIRETION	TESTED WIND DIRECTION
0	0
90	91
180	179
270	270

Calibrated by :

Mr. W

Mechanical Engineer

Calibration & Test Section

Meteorological Instruments B

Envisat Co., Ltd.

รับรองสำเนาถูกต้อง
ผู้จัดการฝ่ายควบคุมคุณภาพ



THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804,0-2399-0469

The Result of Calibration

Sensor model

EWSNV110WS2503

Certification No. 172/24

6 April, 2024

Page : 3 of 6

Standard Barometer	Tested Barometer	Correction
Pressure	Pressure	
1009.59	1010.02	-0.43
1009.45	1009.95	-0.50
1010.10	1010.53	-0.43
1010.94	1011.36	-0.42
1011.46	1011.85	-0.39
1011.84	1012.34	-0.50
1012.06	1012.47	-0.41
1013.04	1013.48	-0.44
1013.18	1013.56	-0.38
1012.89	1013.27	-0.38
1013.20	1013.61	-0.41
1013.44	1013.85	-0.41
1013.81	1014.21	-0.40
1014.19	1014.68	-0.49
1015.96	1016.32	-0.36
1016.23	1016.65	-0.42
1015.64	1016.03	-0.39
1015.23	1015.68	-0.45
1012.87	1013.31	-0.44
1013.63	1014.10	-0.47

Average

Calibrated by :

Mr. Wa

Mechanical Engineer

Calibration & Test Section

Meteorological Instrument



รับรองสำเนาถูกต้อง
ผู้จัดการฝ่ายควบคุมคุณภาพ



THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804, 0-2399-0469

The Result of Calibration

Sensor model

EWSNV110WS2503

Certification No. 172/24

6 April, 2024

Page : 4 of 6

Standard Temp. °C	Temperature Sensor Reading	
	Reading °C	Correction °C
45.6	46.0	-0.4
30.1	30.3	-0.2
15.4	15.7	-0.3

Calibrated by :

Mr. W

Mechanical Engineer

Calibration & Test Section
Meteorological Instruments Bureau



รับรองสำเนาถูกต้อง
ผู้ให้การฟ่ายควบคุมคุณภาพ



THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804,0-2399-0469

The Result of Calibration

Sensor model EWSNV110WS2503 Certification No. 172/24

6 April, 2024

Page : 5 of 6


Standard Humidity % R.H.	Relative Humidity Sensor Reading	
	Reading % R.H.	Correction % R.H.
85.2	91.5	-6.3
62.4	67.7	-5.3
41.5	46.2	-4.7

Calibrated by

M

Mechanical Engineer

Calibration & Test Section
Meteorological Instruments Bureau



รับรองสำเนาถูกต้อง
ผู้ตรวจพิจารณาคุณภาพ



Date of Issue 6 April, 2024

Certification No. 172/24

Page: 6 of 6

ใบรับรอง

หนังสือฉบับนี้ขอรับรองว่า เครื่องวัดฝน ยี่ห้อ Davis Instruments แบบ TIPPING
BUCKET Product No. #7852 Mfg. Code. EWSNV110WS2503 ทำการสอบเทียบกับแก้ววัดฝน
แบบแก้วดวง GAUGE DIAMETER 8.0 INCHES, NEGRETTI & ZAMBRA LONDON No.
71082 และสามารถนำไปใช้ได้ มีค่าถูกต้องตามรายละเอียดของเครื่องมือ (0.2 mm./TIP)



ลงชื่อ...

(นายวัชรพล ทรัพย์วัฒน)

วิศวกรชำนาญการ



รองศาสตราจารย์ ดร. อดิศักดิ์ ตรีเวทย์
ผู้อำนวยการศูนย์ทดสอบคุณภาพ



THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-67/0391

MTC No. EEL. BP. 30/0467

CALIBRATION CERTIFICATE

Submitted by : Envilab Co.,Ltd.

Address : 540, 540/1 Soi Bangkhuae 7, Bangkhuae, Bangkhuae, Bangkok 10160.

Calibrated at : Electrical and Electronic Standards Laboratory, Industrial Metrology and Testing Service Centre.
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Rd., Muang, Samutprakan 10280.

Instrument Calibrated :

Description : Sound Level Calibrator

Manufacturer : Bruel & Kjaer

Model : 4230

Serial No. : 1351075

Ambient Environment

Temperature : $(23 \pm 3) ^\circ\text{C}$

Relative Humidity : $(50 \pm 15) \%$

Ambient Pressure : $(101.325 \pm 1.500) \text{ kPa}$

- Standards used :
1. Digital Function Synthesizer NF Electronic DF-193A S/N 122037.
 2. Measuring Amplifier Bruel&Kjaer 2636 S/N 1537484.
 3. Programmable Attenuator Tamagawa TPA-303A S/N OF 2214.
 4. Digital Multimeter Agilent 34401A S/N MY44005560.
 5. Pressure Transmitter Vaisala PTB202AD S/N T0650001.
 6. Audio Analyzer Keithley 2015-P S/N4106495.
 7. Condenser Microphone B&K 4180 S/N 2889871.

Calibration Procedure: CP-102-04 based on IEC 60942-2003; The sound pressure level generated by sound calibrator under test shall be measured by standard microphone using an insert voltage technique.

This instrument has been calibrated against standards maintained at Electrical and Electronic Standards Laboratory (EEL), which are traceable to the International System of Units through the National Institute of Metrology (Thailand).

The information on actual reading is attached herewith and the uncertainty limits quoted refer to the measured values only.

Date of Receipt : 9 Apr. 2024

Date of Calibration : 10 Apr. 2024

1 / 2

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

Head Office

35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9009

Office/Laboratory

668 Mu 2 Tambon Bangpoomai, Amphoe Muang Samutprakan,
Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtc@tistr.or.th Website : www.tistr.or.th



Envilab Co., Ltd. ผู้ให้บริการด้านความคุ้มครองคุณภาพ



THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-67/0391

MTC No. EEL. BP. 30/0467

The reported expanded uncertainty is based upon a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%.

Nominal Output of Unit Under Test = 94 dB re 20 μ Pa at 1000 Hz

Acoustic Output in dB re 20 μ Pa, Corrected to Reference Conditions: 101.325 kPa, 23.0 °C and 50 %RH.

1. Sound Pressure Level

Standard Microphone Type	Measured Sound Pressure Level (dB)	Deviated value (dB)	Uncertainty (dB)	Tolerance limit IEC60942:2003 Class 1
1/2 inch Bruel&Kjaer 4180	93.72	-0.28	± 0.10	± 0.40 dB

2. Frequency

Standard Microphone Type	Measured Frequency (Hz)	Deviated value (Hz)	Uncertainty (Hz)	Tolerance limit IEC60942:2003 Class 1
1/2 inch Bruel&Kjaer 4180	994.9	-5.1	± 1.5	$\pm 1.0\%$

3. Total Distortion

Standard Microphone Type	Measured Total Distortion (%)	Uncertainty (%)	Tolerance limit IEC60942:2003 Class 1
1/2 inch Bruel&Kjaer 4180	1.25	± 0.50	$\pm 3.0\%$

Note : 1. No adjustment.

2. The calibrator pressure correction was not included.

3. The microphone volume correction was not included.

Calibrated by :

.....
(M.....e)

Approved by :



Director
TISTR

Electrical and Electronic Standards Laboratory

Industrial Metrology and Testing Service Centre

Date of Calibration : 10 Apr. 2024

Date of Issue : 11 Apr. 2024

Ref : 2011267040901374001

End of Certificate

2 / 2

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

Head Office

35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9009

Office/Laboratory

668 Mu 2 Tambon Bangpoomai, Amphoe Muang Samutprakan,
Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtc@tistr.or.th Website : www.tistr.or.th

Office

196 Phanomyoth
Bangkok 10900,
Tel. (66) 0 2579 1121-30 ext. 6219, 6225, 6217
(66) 08-1889-6827



Envilab Co., Ltd.

ผู้จัดการฝ่ายควบคุมคุณภาพ



บริษัท เอ็นไวเล็บ จำกัด 540,540/1 ซอยบางแค 7 แขวงบางแค เขตบางแค กรุงเทพฯ 10160
EnviLab Co., Ltd. 540,540/1 Soi Bangkhae 7 Bangkhae Bangkok Bangkok 10160
Tel : 02-802-3577-8 Fax. 02-802-3773 E-mail : info@evltesting.com



EnviLab & Noxide Supply Instrument

TSP High Volume Sampler Calibration

Verification Report No.

SO2400034-E012 -TSP 01

☐ PM ☒ Onsite

Site: โรงเรียน รัดนัฏ

UTM : N 1777870 E 251653

Sampler: ETSP#35

Recorder: ECRAN000031070

Date: 12 Nov 24

Technical: PANLOP PROMMEE

Approval: Wisan Ritthikamon

CONDITIONS

Barometric Press. (hPa): 990.3

Temperature (deg C): 32.0

Average Press. (hPa): 990.0

Average Temp. (deg C): 31.0

Corrected Pressure (mm Hg): 742.8

Temperature (deg K): 305.0

Corrected Avg. Press. (mm Hg): 742.6

Average Temp. (deg K): 304.0

CALIBRATION ORIFICE

Brand: Tisch Environmental, Inc

Model: TE-5025A

Serial#: 5411

Qstd Slope: 2.02024


Qstd Intercept: -0.02667

Date Certified: 9 Feb 2024

Due Date : 08-Feb-25

CALIBRATIONS

Plate or Test #	H2O (in)	Qstd (m3/min)	I (chart)	IC (corrected)	LINEAR REGRESSION
1	12.80	1.744	58.0	56.68	Slope = 32.4201
2	9.70	1.520	52.0	50.81	Intercept = 0.5954
3	7.30	1.320	44.0	43.00	Corr. coeff.= 0.9988
4	4.80	1.073	36.0	35.18	
5	2.80	0.823	28.0	27.36	
					# of Observations: 5
					Range of Chart at 1.1 - 1.7 m3/min. 38 57

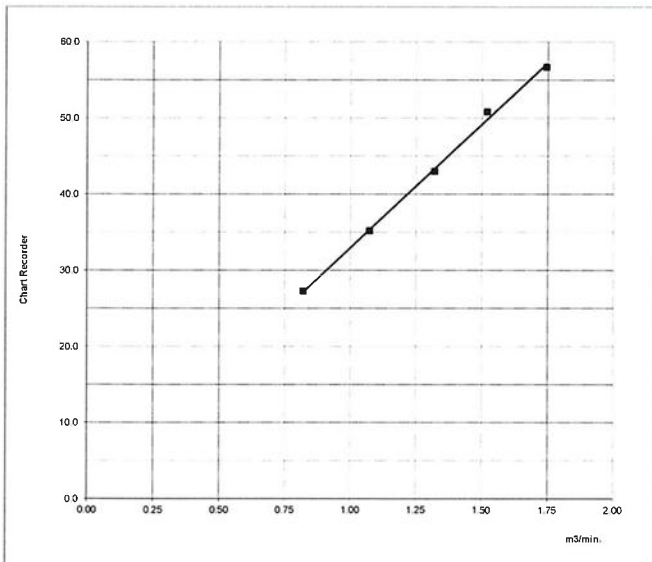

Calibrated by :

12 November 2024

Approved by :

This report shall not be reproduced except in full, without the written approval of EnviLab Co., Ltd.

www.evltesting.com

Environmental responsibility with accuracy measurement

FE-MNT-29 Rev.02.05/07/67



รับรองสำเนาถูกต้อง
ผู้ดำเนินการตรวจสอบ



บริษัท เอ็นไวแล็บ จำกัด 540,540/1 ซอยบางแค 7 แขวงบางแค เขตบางแค กรุงเทพฯ 10160
Envilab Co., Ltd. 540,540/1 Soi Bangkhoe 7 Bangkhoe Bangkok Bangkok 10160
Tel : 02-802-3577-8 Fax. 02-802-3773 E-mail : info@evltesting.com



Envilab & Newtest Supply Instrument

PM10 High Volume Sampler Calibration

Verification Report No.

SO2400034-E012 -PM 01

☐ PM ☒ Onsite

Site: โรงเรียน รัดมนัฒ

UTM : N 1777870 E 251653

Sampler: EPM10#44

Recorder: EVFCDPR02TC004

Date: 12 Nov 24

Technical: PANLOP PROMMEE

Approval: Wisan Ritthikamon

CONDITIONS

Barometric Press. (hPa): 990.3

Temperature (deg C): 32.0

Average Press. (hPa): 990.0

Average Temp. (deg C): 31.0

Corrected Pressure (mm Hg): 742.8

Temperature (deg K): 305.0

Corrected Avg.Press. (mm Hg): 742.6

Average Temp. (deg K): 304.0

CALIBRATION ORIFICE

Brand: Tisch Environmental, Inc

Model: TE-5025A

Serial#: 5411

Qstd Slope: 1.2654


Qstd Intercept: -0.01667

Date Certified: 9 Feb 2024

Due Date : 08-Feb-25

CALIBRATIONS

Plate or Test #	H2O (in)	Qa (m3/min)	I (chart)	IC (corrected)	LINEAR REGRESSION
1	12.30	1.789	54.0	34.60	Slope = 17.5200
2	9.40	1.566	46.0	29.48	Intercept = 2.8692
3	7.10	1.363	42.0	26.91	Corr. coeff. = 0.9962
4	4.80	1.123	36.0	23.07	SFR = 1.133
5	2.90	0.876	28.0	17.94	SSP = 35.47
					# of Observations: 5
					Range of Chart at SFR $\pm 10\%$
					33
					38

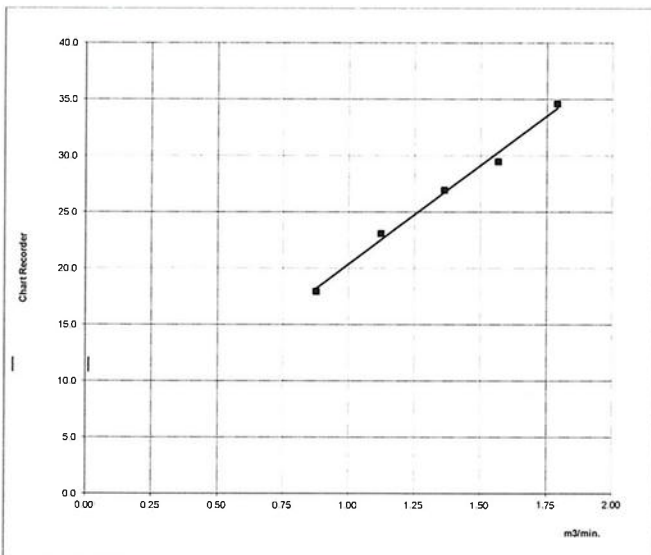

Calibrated by :

PANLOP PROMMEE
12 November 2024

Approved by :

12 November 2024

This report shall not be reproduced except in full, without the written approval of Envilab Co., Ltd.

www.evltesting.com

Environmental responsibility with accuracy measurement

FE-MNT-29 Rev 02/05/07/07



รับรองสำเนาถูกต้อง
ผู้ลงนามฝ่ายควบคุมคุณภาพ



บริษัท เอ็นไวแล็บ จำกัด 540,540/1 ซอยบางแค 7 แขวงบางแค เขตบางแค กรุงเทพฯ 10160
Envilab Co., Ltd. 540,540/1 Soi Bangkhae 7 Bangkhae Bangkhae Bangkok 10160
Tel : 02-802-3577-8 Fax. 02-802-3773 E-mail : info@evltesting.com



Envilab & Neediss Supply Instrument

Verification Test Report

Report No.:

SO2400034-E012 -SLM 01

☐ PM ☒ Onsite UTM : N 1777851 E 251634

Calibrated Date: 12 November 2024

Site : โรงเรียน รัตนจักร

Equipment: Sound Level Meter

Manufacturer: PULSAR

Model: 44

Serial : 2199

Environment: Temperature 33 °C Humidity 56 %RH

Reference Standard: Acoustic Calibrator Class 1 Model 4230, Bruel&Kjaer

Serial No.1351075

Date of Calibration : 10 Apr 2024

Uncertainty : 0.10 dB

Result of Test

Reference Standard (dB)	Instrument reading (dB)	Error (dB)	Adjust (dB)
93.80	93.90	0.10	93.80
Error After Adjust (dB)	Total Error (dB)	Acceptant value	Pass/Fail Judgment
0.00	0.10	±1.0 dB	Pass

Calibrated By:

([Redacted Signature])

Date: 12 November 2024

Approve By:

([Redacted Signature])
(Wisan Ritthikamon)

Date: 12 November 2024

This report shall not be reproduced except in full, without the written approval of Envilab Co., Ltd.



บริษัท เอ็นไวแล็บ จำกัด 540,540/1 ซอยบางแค 7 แขวงบางแค เขตบางแค กรุงเทพฯ 10160
Envilab Co., Ltd. 540,540/1 Soi Bangkhae 7 Bangkhae Bangkhae Bangkok 10160
Tel : 02-802-3577-8 Fax. 02-802-3773 E-mail : info@evltesting.com



Envilab & Needless Supply Instrument

Verification Test Report

Report No.:

SO2400034-E012 -SLM 02

☐ PM ☒ Onsite UTM : -

Calibrated Date: 12 November 2024

Site : ภายในพื้นที่คลังน้ำมัน

Equipment: Sound Level Meter

Manufacturer: PULSAR

Model: 44

Serial : 2197

Environment: Temperature 33 °C Humidity 56 %RH

Reference Standard: Acoustic Calibrator Class 1 Model 4230, Bruel&Kjaer
Serial No.1351075
Date of Calibration : 10 Apr 2024
Uncertainty : 0.10 dB

Result of Test

Reference Standard (dB)	Instrument reading (dB)	Error (dB)	Adjust (dB)
93.80	93.70	-0.10	93.80
Error After Adjust (dB)	Total Error (dB)	Acceptant value	Pass/Fail Judgment
0.00	0.10	±1.0 dB	Pass

Calibrated By:

([REDACTED])

Date:

12 November 2024

Approve By:

([REDACTED])

Date:

12

This report shall not be reproduced except in full, without the written approval of Envilab Co., Ltd.

Envilab Co., Ltd.

ลงนามถูกต้อง

ผู้ตรวจการฝ่ายควบคุมคุณภาพ



neediss

บริษัท นีดีส ซัพพลาย อินสตรูमेंท์ จำกัด
Neediss Supply Instrument Co., Ltd.

536 ซอยบางแค 7 แขวงบางแค เขตบางแค กรุงเทพมหานคร 10160 536 Soi Bangkhae 7 Bangkhae Bangkok
Tel. 02-302-3960-2 Fax. 02-302-3988 Email: info@neediss.com



SO2 Analyzer Verification Test Report

Calibration Report No.: AP-S6711001

Calibrated Date: 6-Nov-24

☒ PM ☐ Onsite

Page: 1/2

Instruments Information

Analyzer Type: SO2 Analyzer Model: 100A	Manufacturer API S/N: ESOAIT10002034
--	---

Calibration System


Calibrator Unit	Standard Gas
Dilutor Model ESA MGC101 S/N: 792 ZERO AIR Generator ZAG7001 S/N: 644	NOx Conc 46.50 PPM NO Conc 46.50 PPM SO2 Conc 45.59 PPM CO Conc 4507 PPM Expire Date: Mar 31, 2026 EB0160267

Environment: Temperature 27.9 °C

Humidity: 74 %RH

Calibration Report

Status	Zero			Span		
	Reference (ppb)	Reading (ppb)	Drift (ppb)	Reference (ppb)	Reading (ppb)	Drift%
Before	0.0	1.3	1.3	400.0	408.1	1.0
After	0.0	0.7	0.7	400.0	404.0	0.5

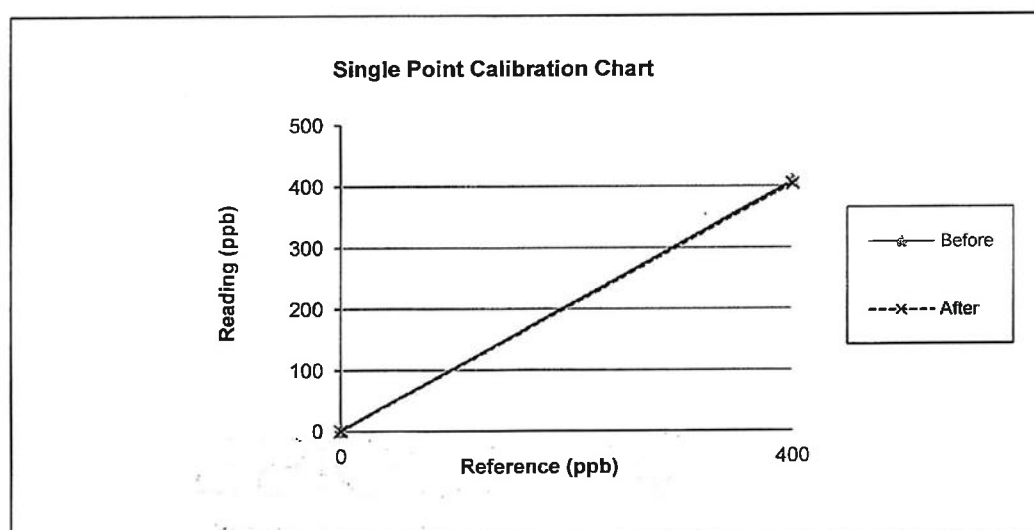



SO2 Analyzer Verification Test Report

Calibration Report No.: AP-S6711001

Calibrated Date: 6-Nov-24

☒ PM ☐ Onsite

Page:2/2

Test Function Value	Normal range	Unit	Before	After	Note
Date	6-Nov-24				
Time	010:30:00				
Range	50 - 20000	PPB	500	500	
Stability (Zero Gas)	< 0.2	PPB	0.4	0.2	
Sample Flow	650 (+/- 50)	cc/min	666	662	
PMT Detector	0 - 5000	mV	24.3	28.2	
Norm PMT Detector	0 - 5000	mV	31.4	34.3	
HVPS	400-900 constant	V	725	725	
DCPS	2500 (+/- 200)	mV	-	-	
RCCELL TEMP	50 (+/- 1)	Dreegee C	50	50	
BOX TEMP	20-40	Dreegee C	32.6	35.1	
PMT TEMP	7 (+/-1)	Dreegee C	8.3	8.3	
UV lamp	1000-4900	mV	3251	3251	
Lamp Ratio	30-120	%	87.4	87.4	
STR. Light (Zero Gas)	<100	PPB	38.5	38.5	
Dark PMT	(-50) - (+200)	mV	27.6	27.6	
Dark lamp	(-50) - (+200)	mV	3.6	3.6	
SAMP PRES	20-30 contant	IN-Hg-A	26.9	27.3	
Electric Test/Optic Test					
PMT Volts	2000 (+/- 500)	mV	2010	2006	
SO2 Conc	1000 (+/- 250)	PPB	1005	1003	
SO2 Slope	1 (+/- 0.3)	-	1.054	1.053	
SO2 Offset	< 250	mV	94.7	90.4	
Stability at Zero	< 0.2	PPB	0.1	0.1	
Stability at Span	< 2 ppb @ 400 ppb	PPB	0.4	0.2	
Gas Test Response					
Zero Gas (0.00 PPB)	0	ppb	1.3	0.7	
Span Gas (400 PPB)	400	ppb	408.1	404.0	± 5% of Range

Calibrate By : _____

Date:

6-Nov-24

Approve By : _____

Date:

6-Nov-24


neediss
 Neediss Supply Instrument Co., Ltd





NOx Analyzer Verification Test Report

Calibration Report No.: AP-N6711001

Page:1/1

Calibrated Date: 1-Nov-24

☒ PM
 ☐ Onsite

Page:2/2

Test Function Value	Normal range	Unit	Before	After	Note
Date	1-Nov-24				
Time	9:25				
Range	0.00 - 500.00 PPB	PPB	500	500	
Stability (Zero Gas)	< 0.2	PPB	0.5	0.2	
Sample Flow	500+/- 50	cc/min	491	485	
Ozone Flow	60-90	cc/min	80	80	
PMT Detector	0-5000	mV	85.0	25.0	
AZERO	-20-150	mV	94.1	14.5	
HVPS	400-900 constant	V	734	734	
DCPS	2500 +/- 200	mV	-	-	
RCELL TEMP	50+/- 1	Dreegee C	50	50	
BOX TEMP	20-35	Dreegee C	34.7	33.6	
PMT TEMP	7 +/-1	Dreegee C	7.0	7.0	
IZS TEMP	50+/- 4	Dreegee C	-	-	
MOLY Temp	315 +/- 5	Dreegee C	314.0	314.0	
RCEL PRES	4-10 contant	IN-Hg-A	5.0	5.0	
SAMP PRES	20-30 contant	IN-Hg-A	28.8	27.9	
NO Slope	1 +/- 0.3		1.135	1.197	
Nox Slope	1 +/- 0.3		1.260	1.114	
NO Offset	-10 to + 150	mV	0.8	-3.6	
NOx Offset	-10 to + 150	mV	-2.6	6.1	
Span and Cal Values					
Zero Value	NO	0	ppb	2.3	0.5
	NOx	0	ppb	2.6	0.8
Span Value	NO	400	ppb	390.2	401.0
	NOx	400	ppb	396.0	403.0

Calibrate By : _____

Approve By : _____

Date: _____

1-Nov-24

Date: _____


neediss
 Neediss Supply Instrument Co., Ltd.



EnviLab Co., Ltd. ผู้ตรวจวิเคราะห์คุณภาพ

Certificate of Calibration

Certificate No. : 67-420034-1

Page : 1 of 2

Submitted by : Envilab Co., Ltd.
540,540/1 Soi Bangkhae7, Bangkhae, Bangkok 10160

Equipment : pH Meter with electrode
pH meter
Manufacturer : Horiba Model : F-74BW-G
Range : N/A pH Resolution : 0.001 pH
Serial No. : B41J0001 ID No. : ELABPHHB74BW01
Electrode
Model : 9615S Serial No. : 9X1K0003

Environment : On site calibration was carried out at the Laboratory, Envilab Co., Ltd.
Ambient Temperature : (22.0 to 23.0)° C
Relative Humidity : (50 to 55) %

Date of Received : 20 March 2024

Date of Calibration : 20 March 2024

Date of Issue : 23 March 2024

Calibrated by : Permpoon Chanpu

Calibration Method : In-house method CAL-M4201 direct measurement by using standard voltage calibrator and using certified reference material (CRM)

Reference Standard Instruments : This certification is traceable to the International System of Units

1. Multiproduct Calibrator

ID No.	Cert. No.	Due Date	Traceability
400005	SG-E-00307/66	23 Aug 2025	National Institute of Metrology Thailand (NIMT)

2. Standard Buffer Solution

pH	Cert. No.	Lot No.	Exp. Date	Traceability
4.008	61293328	944535	27 Nov 2025	CPA Chem Ltd. Accredited to ISO 17034 and ISO/IEC 17025
6.986	61281486	944537	17 Nov 2024	CPA Chem Ltd. Accredited to ISO 17034 and ISO/IEC 17025
9.997	61281073	944536	17 Nov 2024	CPA Chem Ltd. Accredited to ISO 17034 and ISO/IEC 17025

Approved

(Surachai Promthong)

Laboratory Manager

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.

Certificate of Calibration

Certificate No. : 67-420034-1

Page : 2 of 2

Result of Calibration :

UUC Condition As-Received : Good

Function : Electrical measurement

pH meter

Performing standard curve by Multiproduct Calibrator at pH (4,7,10)

Adjustment Curve at nominal pH	Applied Voltage (mV)	Nominal Value (pH)	UUC Reading		Correction (mV)	Uncertainty (± mV)
			(pH)	(mV)		
4, 7, 10	177.4800	4	3.998	177.5	0.0	0.12
	0.0000	7	7.000	0.0	0.0	0.086
	-177.4800	10	10.000	-177.4	-0.1	0.12

Function : pH meter with electrode

Performing a three - buffer standard curve using buffer nominal pH (4,7,10)

Adjustment Curve at nominal pH	Standard Buffer (pH)	UUC Reading (pH)	Correction (pH)	Uncertainty (± pH)
4, 7, 10	4.008	4.009	-0.001	0.0084
	6.986	7.000	-0.014	0.0092
	9.997	10.008	-0.011	0.014


Remark

UUC : Unit Under Calibration

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurment was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

- o0o -



Certificate of Calibration

Certificate No. : 67-400167-1

Page : 1 of 2

Submitted by : Envilab Co., Ltd.

540,540/1 Soi Bangkhae7, Bangkhae, Bangkok 10160

Equipment : Temperature Indicator with Thermistor Probe

Temperature Indicator

Manufacturer : Horiba

Model : F-74BW-G

Range : N/A °C

Resolution : 0.1 °C

Serial No. : B41J0001

ID No. : ELABPHHB74BW01

Thermistor probe

Model : 9615S

Sheath Material : Glass

Diameter : 12 mm.

Length : 151 mm.

Serial No. : 9X1K0003

ID No. : ELABPHHB74BW01

Environment : On site calibration was carried out at the Laboratory, Green Earth Environment Co., Ltd.

Ambient Temperature : (22.0 to 23.0) °C

Relative Humidity : (50 to 55) %

Line Voltage : (220.0 to 223.0) VAC

Date of Received : 20 March 2024

Date of Calibration : 20 March 2024

Date of Issue : 23 March 2024

Calibrated by : Permpon Chanpu

Calibration Method : This instrument was calibrated by In-house method comparison technique CAL-M4003 by compared with PRT in the liquid bath at the constant controlled temperature.

The temperature scale used was based on ITS-90

Reference Standard Instruments : This certification is traceable to the International System of Units

1. Platinum Resistance Thermometer (PRT)

ID No.	Cert. No.	Due Date	Traceability
400002	TT-0074-22	20 Jun 2024	National Institute of Metrology Thailand (NIMT)

2. Standard Digital Thermometer

ID No.	Cert. No.	Due Date	Traceability
400003/400004	23E1866	01 Jun 2025	National Institute of Metrology Thailand (NIMT)

Approved by

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Envilab Co.,Ltd.

การรับรองการสอบเทียบ
การสอบเทียบ



CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhaprachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech.cal@yahoo.com, calibratech.cal@hotmail.com

Certificate of Calibration

Certificate No. : 67-400167-1

Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Function : Temperature measurement

Immersion Depth (mm.)	Standard Reading (°C)	UUC Reading (°C)	Correction (°C)	Uncertainty (± °C)
130	25.002	25.0	0.0	0.19

Remark

UUC : Unit Under Calibration

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

- o0o -



รับรองสำเนาถูกต้อง
ผู้ลงนามฝ่ายควบคุมคุณภาพ





MIRACLE INTERNATIONAL TECHNOLOGY CO.,LTD

214 Bangwack Rd. Bangpai Bangkhae Bangkok 10160
Tel.: 0-2865-4647-8 Fax: 0-2865-4649 <http://www.mit.in.th>



CALIBRATION CERTIFICATE

Certificate No. : S2024040558-0002

Date Issued : 03-May-24

Customer : Envilab Co., Ltd.
540, 540/1 Soi Bangkhae 7, Bangkhae, Bangkok, Thailand
10160

Equipment : Lab Refrigerator (TMF-PLR221)

Manufacturer : Thermo Scientific

Model : PLR221

Serial No. : 2210M319042801

ID No./Tag No. : ELABREFRIGEN02

Date Received : 02-May-24

Date Calibrated : 02-May-24

Calibrated by : Mr. Varuch Jearrajinda

Calibration Method or Calibration Procedure Used


Standard method : CP-05 TLAS G-20.

This certificate is traceable to national standards, which realize the units of measurement according to the International System of Units (SI).

Result of Calibration

The reported uncertainty of measurement was based on standard uncertainty multiplied by a coverage factor $k = 2$, providing a level confidence approximately 95 percent.

This certificate may not be reproduced other than in full except with the prior written approval of the Miracle International Technology Company Limited.

Approved by: 

(Mr. Varuch Jearrajinda)



Page 1 of 2



ได้รับรองจากหน่วยงาน
ผู้ให้การรับรองคุณภาพ

Certificate No. : S2024040558-0002

Environment : Ambient Temperature : Start record 26.6 °C, Stop record 26.8 °C
Relative Humidity : Start record 54.1 %RH, Stop record 54.5 %RH

Calibration Temperature (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Stability ¹ (°C)	Measured Uniformity ² (°C)	Overall Variation ³ (°C)
4	4	4	0.88	0.69	1.94

Without adjustment

Calibration Temperature (°C)	STD No. 1 (°C)	STD No. 2 (°C)	STD No. 3 (°C)	STD No. 4 (°C)	STD No. 5 (°C)	STD No. 6 (°C)	STD No. 7 (°C)	STD No. 8 (°C)	STD No. 9 (°C)	Uncertainty ⁴ (±°C)
4	4.23	4.35	4.44	4.46	4.35	4.24	4.34	3.96	4.13	1.2

Decision Rule with Guard Band


Calibration Temperature (°C)	No. 1	No. 2	No. 3	No. 4	No. 5	No. 6	No. 7	No. 8	No. 9	MPE (±°C)
4	Pass	Pass	Pass	Pass	Pass	Pass	Pass	Pass	Pass	2

Pass = $|\text{error}| + |\text{uncertainty}| \leq |\text{MPE}|$ MPE = Maximum Permissible Error

Fail = $|\text{error}| + |\text{uncertainty}| > |\text{MPE}|$

Note : Probe No. 9 is Reference Probe

Setting Air Fresh No. 0



Condition As-Received : Used Item

The measurement results and statements of conformity with specification only relate to the item calibrated.

Measurement Standards Used & Traceability :

The International System of Units (SI) through

MIT Certificate No. L202403007-0012 for Digital Thermometer with Probe (Agilent) Module 1 (93) Serial No. MY41008700, Due 10-Sep-24

Notes : 1. The temperature stability is the one-half of greatest maximum difference of measured temperatures at any one probe.

2. The temperature uniformity is the maximum difference of measured temperatures between of any probes and the measured temperature at the reference location which are observed at same time.

3. Overall variation is the difference of maximum and minimum measured temperatures throughout observation time.

4. The uncertainty of measurement is included temperature stability.

5. The temperature uniformity, stability, overall variation and indicating temperature is applicable to all air or gas filled temperature controlled enclosures at atmospheric pressure.

End of Certificate



ข้าราชการนาฎกตอง
นางสาวนันทนาภรณ์

CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhprachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech_cal@yahoo.com, calibratech_cal@hotmail.com



NSC-TISI-TIS17025
CALIBRATION 0030

Certificate of Calibration

Certificate No. : 67-400166-1

Page : 1 of 2

Submitted by : Envilab Co., Ltd.
540, 540/1 Soi Bangkhae 7, Bangkhae, Bangkok 10160

Equipment : Temperature controlled enclosure (Oven)
Manufacturer : Memmert
Model : UF 75
Range : N/A °C
Resolution : 0.1 °C
Serial No. : B319.0600
ID No. : ELABHAOVEN0600

Environment : On site calibration was carried out at the Laboratory, Envilab Co., Ltd.

Ambient Temperature : (29.0 to 30.0) °C

Relative Humidity : (60 to 650) %

Line Voltage : (224.2 to 225.2) V

Date of Received : 20 March 2024

Date of Calibration : 20 March 2024

Date of Issue : 22 March 2024

Calibrated by : Kittisak Kokaeo

Calibration Method : CAL-M4004, TLAS G-20

The temperature scale used was based on ITS-90

Reference Standard Instruments : This certification is traceable to the International System of Units

Standard Digital Thermometer with Thermocouple probe

<u>ID No.</u>	<u>Cert. No.</u>	<u>Due Date</u>	<u>Traceability</u>
400046 & 400028	66-400547-3	05 Apr 2024	National Institute of Metrology Thailand (NIMT)

Approved by

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 67-400166-1


Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Function : Temperature measurement

This instrument was setting air ventilation at position 0 (close)

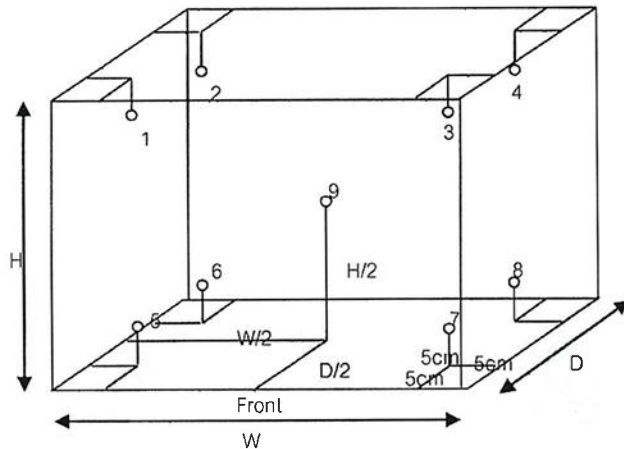

Inside of Chamber

W = 0.40 m

D = 0.33 m

H = 0.56 m

Capacity = 0.07 m³

Test Point (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Temperature (°C) @ Sensor No.									Uncertainty (± °C)
			1	2	3	4	5	6	7	8	9	
104.0	103.5	103.5	104.1	104.4	104.1	104.3	104.1	104.0	104.0	103.7	104.3	0.70
110.0	109.5	109.5	110.1	110.4	110.1	110.3	110.2	110.1	110.1	109.4	110.3	0.72
180.0	179.0	179.0	179.5	180.9	180.3	180.6	180.5	180.3	180.2	180.2	180.8	0.95

Test Point (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Uniformity (°C)	Measured Stability (°C)	Overall Variation (°C)
104.0	103.5	103.5	0.7	0.1	1.0
110.0	109.5	109.5	1.1	0.1	1.2
180.0	179.0	179.0	1.5	0.2	1.6

Remark The uncertainty is not combine uniformity of the air chamber

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k = 2 , providing a level of confidence of approximately 95%

- ๐0๐ -



EnviLab Co., Ltd.

รับรองสำเนาถูกต้อง
ผู้จัดการฝ่ายควบคุมคุณภาพ



CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhaphrachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech_cal@yahoo.com, calibratech_cal@hotmail.com



NSC-TISI-TIS17025
CALIBRATION 0030

Certificate of Calibration

Certificate No. : 67-400166-2

Page : 1 of 2

Submitted by : Envilab Co., Ltd.
540, 540/1 Soi Bangkhac 7, Bangkhac, Bangkok 10160

Equipment : Water Bath
Manufacturer : Memmert Model : WNB 14
Range : N/A °C Resolution : 0.1 °C
Serial No. : L412.2222 ID No. : ELABWBWNB29N01

Environment : On site calibration was carried out at the Laboratory, Envilab Co., Ltd.

Ambient Temperature : (29.0 to 30.0) °C
Relative Humidity : (60 to 65) %
Line Voltage : (224.2 to 225.2) V

Date of Received : 20 March 2024

Date of Calibration : 20 March 2024

Date of Issue : 22 March 2024

Calibrated by : Kittisak Kokaeo

Calibration Method : This instrument was calibrated by In-house method CAL-M4006 based on ASTM E715-80
The temperature scale used was based on ITS-90

Reference Standard Instruments : This certification is traceable to the International System of Units
Standard Digital Thermometer with RTD probe

<u>ID No.</u>	<u>Cert. No.</u>	<u>Due Date</u>	<u>Traceability</u>
400046 & 400024	66-400547-2	02 Apr 2024	National Institute of Metrology Thailand (NIMT)

Approved by

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhprachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech.cal@yahoo.com, calibratech.cal@hotmail.com

Certificate of Calibration


Certificate No. : 67-400166-2

Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Function : Temperature measurement

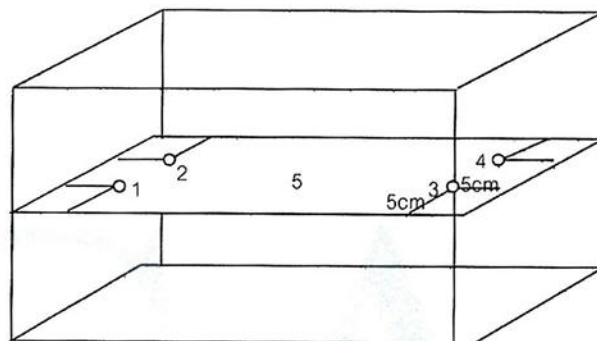

Front

Test Point (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Temperature (°C) @ Sensor No.					Uncertainty (± °C)	Measured Uniformity (°C)	Measured Stability (°C)
			1	2	3	4	5			
95.0	94.5	94.5	95.12	95.18	95.11	95.02	95.17	0.23	0.26	0.12

Remark The uncertainty is not combine uniformity of the water bath

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

- o0o -



รับรองสำเนาถูกต้อง
ผู้รับรองฝ่ายควบคุม



Certificate of Calibration

Certificate No. : 67-200060-1

Page : 1 of 2

Submitted by : Envilab Co., Ltd.
540, 540/1 Soi Bangkhae7, Bangkhae, Bangkok 10160

Equipment : Electronic Balance
Manufacturer : Sartorius Model : SECURA125-1S
Serial No. : 0034606552 ID No. : ELABBALANCEN05
Capacity : 120 g Resolution : 0.0001 g

Environment : On site calibration was carried out at the B304 Balance Room, Envilab Co., Ltd.
Ambient Temperature : (20.0 to 20.7) °C
Relative Humidity : (56.2 to 60.3) %
Air Pressure : 1013.0 mbar

Date of Received : 20 February 2024

Date of Calibration : 20 February 2024

Date of Issue : 21 February 2024

Calibrated by : Satja Sangkhum

Calibration Method : In-house method CAL-M2001 based on UKAS Publication ref : LAB 14
Edition 7 - November 2022

Reference Standard Instruments : This certification is traceable to the International System of Units

Standard Weights

ID No.	Cert. No.	Due Date	Traceability
E261-E2624	C02232088	08 Nov 2024	National Institute of Metrology (Thailand), (NIMT)

Approved by :

Laborat

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co., Ltd.



รับรองสำเนาถูกต้อง
ผู้รับรอง : นายสมชาย งามบุญมา



CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhaphrachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech_cal@yahoo.com, calibratech_cal@hotmail.com

Certificate of Calibration

Certificate No. : 67-200060-1

Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Departure of indication from nominal value

Nominal Value (g)	Correction (g)	Uncertainty \pm (g)
0.1	0.0000	0.00011
0.5	0.0000	0.00011
1	0.0000	0.00011
2	0.0000	0.00011
5	0.0000	0.00011
10	0.0000	0.00011
20	0.0000	0.00013
50	0.0001	0.00014
100	0.0001	0.00020
120	0.0000	0.00038

This result of calibration was found accurate as shown on date and place of calibration only.


This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2.00$, providing a level of confidence of approximately 95%

Eccentric error

Load test : 20 g

A	B	C	D	E
0.0001	0.0001	0.0000	0.0000	0.0000

g



Repeatability

Load test : 100 g

Stdev. : 0.00004 g

- o0o -



Envilab Co.,Ltd.

รับรองสำเนาถูกต้อง

ผู้จัดการฝ่ายควบคุมคุณภาพ



CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhprachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech.cal@yahoo.com, calibratech.cal@hotmail.com



NSC-TISI-TIS 17025
CALIBRATION 0030

Certificate of Calibration

Certificate No. : 67-300293-9

Page : 1 of 2

Submitted by : Envilab Co.,Ltd.

540, 540/1 Soi Bangkhac 7, Bangkhac, Bangkok 10160

Equipment : Cylinder

Manufacturer : Witeg

Class : A

Capacity : 50 ml

Graduation : 1 ml

ID No. : C-HM-001/24

Environment : Ambient Temperature : (20 ± 3) °C

Relative Humidity : (50 ± 10) %

Air Pressure : 1006.0 mbar.

Date of Received : 15 May 2024

Date of Calibration : 20 May 2024

Date of Issue : 20 May 2024

Calibrated by : Areerat Sombun

Calibration Method : In-house method CAL-M3001 based on ASTM E 542-22

Reference Standard Instruments : This certification is traceable to the International System of Units

Electronic Balance

<u>ID No.</u>	<u>Cert. No.</u>	<u>Due Date</u>	<u>Traceability</u>
241002	66-200388-1	02 Jun 2024	National Institute of Metrology (Thailand) (NIMT)

Approved by :



รับรองสำเนาถูกต้อง

Envilab Co.,Ltd. ผู้ดูแลการดำเนินงาน



The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.

CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhaprachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech.cal@yahoo.com, calibratech.cal@hotmail.com

Certificate of Calibration

Certificate No. : 67-300293-9

Page : 2 of 2

Result of Calibration : This result of true Volume is referred to standard temperature at 20 °C

UUC Condition As-Received : Good

Nominal Volume (ml)	Measuring Volume (ml)
25	25.09
50	49.99

Uncertainty of measurement with in \pm 0.054 ml

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2.00$,
providing a level of confidence of approximately 95%

- o0o -



Enviro Co.,Ltd.

รับรองสำเนาถูกต้อง

ผู้จัดการฝ่ายควบคุมคุณภาพ



CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhprachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech.cal@yahoo.com, calibratech.cal@hotmail.com



NSC-TISI-TIS17025
CALIBRATION 0030

Certificate of Calibration

Certificate No. : 67-300147-5

Page : 1 of 2

Submitted by : Envilab Co.,Ltd.

540, 540/1 Soi Bangkhac 7, Bangkhac, Bangkok 10160

Equipment : Cylinder

Manufacturer : PYREX

Class : A

Capacity : 500 ml

Graduation : 5 ml

ID No. : C-WW-005/21

Environment : Ambient Temperature : (20 ± 3) °C

Relative Humidity : (50 ± 10) %

Air Pressure : 1009.3 mbar.

Date of Received : 13 March 2024

Date of Calibration : 19 March 2024

Date of Issue : 19 March 2024

Calibrated by : Areerat Sombun

Calibration Method : In-house method CAL-M3001 based on ASTM E 542-22

Reference Standard Instruments : This certification is traceable to the International System of Units

Electronic Balance

ID No.

Cert. No.

Due Date

Traceability

241002

66-200388-1

02 Jun 2024

National Institute of Metrology (Thailand) (NIMT)

Approved by :



The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.

รับรองสำเนาถูกต้อง

Envilab Co., Ltd.

ผู้จัดการฝ่ายเทคนิค

รับรองสำเนาถูกต้อง



CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhprachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech-cal@yahoo.com, calibratech-cal@hotmail.com

Certificate of Calibration

Certificate No. : 67-300147-5

Page : 2 of 2

Result of Calibration : This result of true Volume is referred to standard temperature at 20 °C

UUC Condition As-Received : Good

Nominal Volume (ml)	Measuring Volume (ml)
250	250.57
500	500.25

Uncertainty of measurement with in \pm 0.12 ml

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2.00$,
providing a level of confidence of approximately 95%

- o0o -



Envilab Co.,Ltd.



รับรองสำเนาถูกต้อง
ผู้จัดการฝ่ายควบคุมคุณภาพ



www.calibratech.co.th

CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhprachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech_cal@yahoo.com, calibratech_cal@hotmail.com



NSC-TISI-TIS17025
CALIBRATION 0030

Certificate of Calibration

Certificate No. : 67-300147-4

Page : 1 of 2

Submitted by : Envilab Co.,Ltd.

540, 540/1 Soi Bangkhac 7, Bangkhac, Bangkok 10160

Equipment : Cylinder

Manufacturer : PYREX

Class : A

Capacity : 250 ml

Graduation : 2 ml

ID No. : C-WW-007/23

Environment : Ambient Temperature : (20 ± 3) °C

Relative Humidity : (50 ± 10) %

Air Pressure : 1009.4 mbar.

Date of Received : 13 March 2024

Date of Calibration : 19 March 2024

Date of Issue : 19 March 2024

Calibrated by : Areerat Sombun

Calibration Method : In-house method CAL-M3001 based on ASTM E 542-22

Reference Standard Instruments : This certification is traceable to the International System of Units

Electronic Balance

<u>ID No.</u>	<u>Cert. No.</u>	<u>Due Date</u>	<u>Traceability</u>
241002	66-200388-1	02 Jun 2024	National Institute of Metrology (Thailand) (NIMT)

Approved by :



รับรองสำเนาถูกต้อง

ผู้จัดการฝ่าย



The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.

CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhprachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech.cal@yahoo.com, calibratech.cal@hotmail.com

Certificate of Calibration

Certificate No. : 67-300147-4

Page : 2 of 2

Result of Calibration : This result of true Volume is referred to standard temperature at 20 °C

UUC Condition As-Received : Good

Nominal Volume (ml)	Measuring Volume (ml)
150	150.31
250	250.38

Uncertainty of measurement with in \pm 0.087 ml

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2.00$,
providing a level of confidence of approximately 95%

- o0o -



Envilab Co.,Ltd.



รับรองว่าถูกต้อง
ผู้จัดทำ: [Signature]



ภาพ

CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhprachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech_cal@yahoo.com, calibratech_cal@hotmail.com



NSC-TISI-TIS17025
CALIBRATION 0030

Certificate of Calibration

Certificate No. : 67-400101-1

Page : 1 of 2

Submitted by : Envilab Co., Ltd.

540, 540/1 Soi Bangkhae 7, Bangkhae, Bangkok 10160

Equipment : Temperature controlled enclosure (Incubator)

Manufacturer : Memmert

Model : IF 75

Range : N/A °C

Resolution : 0.1 °C

Serial No. : D319.0066

ID No. : ELABINCUBATOR2

Environment : On site calibration was carried out at the Laboratory, Envilab Co., Ltd.

Ambient Temperature : (23.0 to 24.0) °C

Relative Humidity : (50 to 55) %

Line Voltage : (223.0 TO 225.0) V

Date of Received : 20 February 2024

Date of Calibration : 20 February 2024

Date of Issue : 22 February 2024

Calibrated by : Kittisak Kokaeo

Calibration Method : CAL-M4004, TLAS G-20

The temperature scale used was based on ITS-90

Reference Standard Instruments : This certification is traceable to the International System of Units
Standard Digital Thermometer with RTD Probe

<u>ID No.</u>	<u>Cert. No.</u>	<u>Due Date</u>	<u>Traceability</u>
400046 & 400047	67-400047-2	26 Jul 2024	National Institute of Metrology Thailand (NIMT)

Approved by

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



ผู้รับรอง : ผู้ตรวจทาน :
Envilab Co.,Ltd. ผู้ตรวจทาน :
www.calibratech.co.th

Certificate of Calibration

Certificate No. : 67-400101-1


Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Function : Temperature measurement

This instrument was setting air ventilation at position 0 (close)

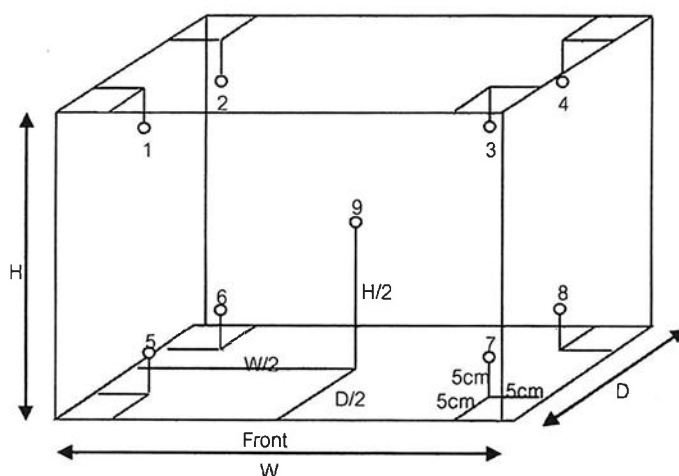

Inside of Chamber

W = 0.40 m

D = 0.56 m

H = 0.33 m

Capacity = 0.07 m³

Test Point (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Temperature (°C) @ Sensor No.									Uncertainty (± °C)
			1	2	3	4	5	6	7	8	9	
35.0	35.3	35.3	34.99	35.13	35.15	35.11	35.08	35.01	34.92	34.91	35.09	0.30
37.0	37.3	37.3	36.96	37.09	37.13	37.08	37.04	36.99	36.90	36.88	37.07	0.30

Test Point (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Uniformity (°C)	Measured Stability (°C)	Overall Variation (°C)
35.0	35.3	35.3	0.2	0.0	0.3
37.0	37.3	37.3	0.2	0.0	0.3

Remark The uncertainty is not combine uniformity of the air chamber

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k = 2 , providing a level of confidence of approximately 95%

- o0o -





SCIMET Co., Ltd.
1194 Soi Wachirathamsathit 57, Bangchak,
Phrakhanong, Bangkok 10260 Thailand
Email:scimet2022@gmail.com, Tel:095-552-4939

Certificate No. C27240001

Calibration Certificate

Equipment: DO METER
Model: HI9147
Serial No.(or ID): H00007030
Manufacturer: HANNA
Condition: In Condition

Job No.: KSMT2400445
Received Date: 04 March 2024
Issued Date: 14 March 2024
Page: 1 of 2

Customer

Envilab Co., Ltd.
540, 540/1 Soi Bangkhae 7, Bangkhae, Bangkok 10160

Calibration Place

Environment Laboratory, SCIMET Co., Ltd.
1194 Soi Wachirathamsathit 57, Bangchak, Prakhnong, Bangkok 10260 Thailand

Calibration Date

14 March 2024

Environment Condition

Temperature: 23 °C \pm 2 °C
Humidity: 50 %RH \pm 15 %RH

The Method used

In-house method, WI27 , By comparison with certified dissolved oxygen solution standard

Traceability

This is certificate is traceable to SI Units , Sample test and temperature test are assured through HANNA instruments company certificare No. 29E31, through Quality Reborn Co.,LTD certificare No.QR23-1169


This certificate is issued the units of measurement according to the International System of Units (SI). It provides traceability of measurement to international or national standard or other recognized national standard laboratories.

The measurement uncertainty stated is the expanded uncertainty which is obtained from the standard uncertainty multiplied by the coverage factor ($k=2$) to provide a level of confidence of approximately 95%. It is determined in accordance with the Guide to Expression of Uncertainty in Measurement (GUM).

These results may be affected by deviations from specified conditions. The results relate only to the items tested, calibrated or sampled. The report shall not be reproduced except in full without approval of SCIMET Co., Ltd.

Mr. Dammong Boonsophon

Person in charge



Mr. Th

รับรองสำเนาถูกต้อง

Envilab Co., Ltd.

ผู้รับบริการ: บริษัท อีวิลแลบ จำกัด

Calibration Results:

Electrode Serial No. KC3N05V1R
Model : H176409
Brand : HANNA

Electrode Test

Atmospheric pressure measured while calibrating. 755.54 mmHg
Temperature measured while calibrating.(± 0.2 °C) 25.0 °C
The Oxygen Solubility was calculated from the ambient conditions. 8.21 \pm 0.03 mg/L
The Oxygen Solubility reading from the DO METER 8.23 mg/L

Sample Test

Standard Oxygen Solution	Unit Under Calibration Reading	Correction	Coverage Factor (<i>k</i>)	Uncertainty of Measurement (\pm)
0.00 mg/L	0.00 mg/L	0.000 mg/L	2.00	0.13 mg/L

Temperature Electrode

Dimension of Probe;

Length : 140 mn.
Diameter : 21 mn.
Immersion Depth 80 mn.

STD. Reading (°C)	UUC. Reading (°C)	Correction of UUC (°C)	Coverage Factor (<i>k</i>)	Uncertainty of Measurement (\pm °C)
25.01	25.0	0.01	2.00	0.15

The End of Certificate



ใบตรวจสอบสภาพเครื่อง Do Meter

เลขที่ใบงาน: KSMT2400445

ชนิดเครื่องมือ: DO METER

รุ่น: HI9147

หมายเลขเครื่อง: H00007030

ตรวจสอบ (รับ)		รายการตรวจเช็ค	ตรวจสอบ (ส่ง)		หมายเหตุ
14 Mar 2024			14 Mar 2024		
ปกติ	ไม่ปกติ		ปกติ	ไม่ปกติ	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	1. ความสมบูรณ์เครื่อง	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	2. ความสะอาด (ช่องใส่ตัวอย่าง, ภายใน-นอกเครื่อง)	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	3. สวิทช์ ปิด – เปิด เครื่อง (On-Off Swicth)	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	4. ปุ่มกด (Keypad)	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	5. หน้าจอ (Display, Screen Contrast)	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	6. อิเล็กโทรด (Electrode and Connection Cable)	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	7. สายอิเล็กโทรด	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	8. เซ็นเซอร์อิเล็กโทรด	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	9. ขาจับอิเล็กโทรด (Stand)	<input checked="" type="checkbox"/>	<input type="checkbox"/>	


ข้อแนะนำ :

Mr.Dumrong Boonsopon

Service Engineer

บริษัท ขายนีเมก จำกัด (SCIMET CO., LTD.)

1194 Soi Wachirathamsathit 57, Bangchak, Phrakhanong, Bangkok 10260 Thailand
Email: scimet2022@gmail.com, Tel: 095 552 4939



รับรองสำเนาถูกต้อง
ผู้จัดการฝ่ายควบคุมคุณภาพ

CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhprachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech-cal@yahoo.com, calibratech-cal@hotmail.com



Certificate of Calibration

Certificate No. : 67-200060-2

Page : 1 of 2

Submitted by : Envilab Co., Ltd.
540, 540/1 Soi Bangkhae7, Bangkhae, Bangkok 10160

Equipment : Electronic Balance
Manufacturer : METTLER TOLEDO **Model :** XSR205DU
Serial No. : B911363567 **ID No. :** ELABBALANCEN06
Capacity : 220 g **Resolution :** 0.00001g/81g, 0.0001g/220g

Environment : On site calibration was carried out at the B304 Balance Room, Envilab Co., Ltd.
Ambient Temperature : (20.0 to 20.5) °C
Relative Humidity : (54.2 to 59.1) %
Air Pressure : 1013.0 mbar

Date of Received : 20 February 2024

Date of Calibration : 20 February 2024

Date of Issue : 21 February 2024

Calibrated by : Satja Sangkhum

Calibration Method : In-house method CAL-M2001 based on UKAS Publication ref : LAB 14
Edition 7 - November 2022

Reference Standard Instruments : This certification is traceable to the International System of Units

Standard Weights

<u>ID No.</u>	<u>Cert. No.</u>	<u>Due Date</u>	<u>Traceability</u>
E261-E2624	C02232088	08 Nov 2024	National Institute of Metrology (Thailand), (NIMT)

Approved by :

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co., Ltd.

CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhprachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech.cal@yahoo.com, calibratech.cal@hotmail.com

Certificate of Calibration

Certificate No. : 67-200060-2

Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Departure of indication from nominal value

Nominal Value (g)	Correction (g)	Uncertainty \pm (g)
0.1	0.00000	0.000015
0.5	0.00001	0.000022
1	0.00000	0.000026
2	0.00001	0.000034
5	-0.00001	0.000043
10	0.00000	0.000053
50	0.00003	0.00011
100	0.0001	0.00020
150	0.0001	0.00038
200	0.0002	0.00038


This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2.00$, providing a level of confidence of approximately 95%

Eccentric error

Load test : 50 g

A B C D E
0.00000 0.00000 0.00010 0.00000 0.00000 g




Repeatability

Load test : 200 g

Stdev. : 0.000032 g

- o0o -





SCIMET Co., Ltd.
1194 Soi Wachirathamsathit 57, Bangchak,
Phrakhanong, Bangkok 10260 Thailand
Email:scimet2022@gmail.com, Tel: 02 460 9239
https://www.scimet.co.th



Certificate No. C07240032

Calibration Certificate

Equipment:

SPECTROPHOTOMETER
Model: CARY 60UV-VIS
Serial No.(or ID): MY17490026 (ELABSPECTRO0002)
Manufacturer: Agilent
Condition: In Condition

Job No.: KSMT2400444
Received Date: 04 March 2024
Issued Date: 04 March 2024
Page: 1 of 3

Customer

Envilab Co., Ltd.
540, 540/1 Soi Bangkhuae 7,Bangkhuae, Bangkhuae, Bangkok 10160

Calibration Place

Envilab Co., Ltd.(B301 CO-THC ROOM)
540, 540/1 Soi Bangkhuae 7,Bangkhuae, Bangkhuae, Bangkok 10160

Calibration Date

04 March 2024

Environment Condition

Temperature: 22.3 °C \pm 0.6 °C
Humidity: 65.7 %RH \pm 0.5 %RH

The Method used

In-house method, WI07, based on ASTM E 275-08 and
ASTM E 387-04

Traceability

This certificate is traceable to the CRM maintained by National Institute
of Standards and Technology (NIST) through Starna Scientific Limited.

The standard for Wavelength Certificate No. 108691 and 108692

The standard for Photometric Certificate No. 109010 , 114655 and 109009

This certificate is issued the units of measurement according to the International System of Units (SI). It provides traceability of measurement to international or national standard or other recognized national standard laboratories.

The measurement uncertainty stated is the expanded uncertainty which is obtained from the standard uncertainty multiplied by the coverage factor ($k=2$) to provide a level of confidence of approximately 95%. It is determined in accordance with the Guide to Expression of Uncertainty in Measurement (GUM).

These results may be affected by deviations from specified conditions. The results relate only to the items tested, calibrated or sampled. The report shall not be reproduced except in full without approval of SCIMET Co., Ltd.

(Mr. Dumrong Boonsopon)

Person in charge



(Mr. [Redacted] am)

Authorized signatory



FC07240032 MAY 2023
ใบรองสำเนา
ผู้ตรวจวัดและควบคุมคุณภาพ


**Calibration Results:****Without Adjustment**

Wavelength Accuracy (nm), The spectral bandwidth of Std at 1.5 nm and UUC at 1.5 nm

Standard Wavelength (nm)	Unit Under Calibration (nm)	Correction (nm)	Uncertainty of Measurement (\pm nm)
219.73	220.0	-0.27	0.14
241.55	241.8	-0.25	0.16
287.56	287.6	-0.04	0.14
333.77	333.7	0.07	0.19
360.45	360.1	0.35	0.14
417.59	417.0	0.59	0.14
472.50	472.3	0.20	0.14
513.47	513.4	0.07	0.14
528.88	528.9	-0.02	0.14
537.18	537.1	0.08	0.14
641.58	642.3	-0.72	0.16
740.72	741.3	-0.58	0.14
748.55	749.1	-0.55	0.14
807.03	807.4	-0.37	0.14
879.28	879.0	0.28	0.14

Photometric Accuracy (Absorbance)

Wavelength	Standard absorbance (Abs)	Unit Under Calibration (Abs)	Correction (Abs)	Uncertainty of Measurement (\pm Abs)
235 nm	0.0000	0.0000	0.0000	0.0080
	0.7293	0.7273	0.0020	0.0080
257 nm	0.0000	-0.0003	0.0003	0.0080
	0.8497	0.8457	0.0040	0.0080
313 nm	0.0000	0.0004	-0.0004	0.0080
	0.2833	0.2810	0.0023	0.0080
350 nm	0.0000	0.0001	-0.0001	0.0080
	0.6299	0.6259	0.0040	0.0080


**Calibration Results:****Without Adjustment****Photometric Accuracy (Absorbance)**

Wavelength	Standard absorbance (Abs)	Unit Under Calibration (Abs)	Correction (Abs)	Uncertainty of Measurement(\pm Abs)
420 nm	0.0000	0.0000	0.0000	0.0045
	0.2373	0.2386	-0.0013	0.0045
	0.5617	0.5637	-0.0020	0.0045
	0.7392	0.7382	0.0010	0.0045
	1.0550	1.0542	0.0008	0.0045
440 nm	0.0000	0.0000	0.0000	0.0045
	0.2335	0.2354	-0.0019	0.0045
	0.5513	0.5539	-0.0026	0.0045
	0.7230	0.7222	0.0008	0.0045
	1.0324	1.0343	-0.0019	0.0045
465 nm	0.0000	0.0000	0.0000	0.0045
	0.2126	0.2143	-0.0017	0.0045
	0.5036	0.5059	-0.0023	0.0045
	0.6735	0.6729	0.0006	0.0045
	0.9615	0.9638	-0.0023	0.0045
546.1 nm	0.0000	0.0000	0.0000	0.0045
	0.2201	0.2213	-0.0012	0.0045
	0.5176	0.5196	-0.0020	0.0045
	0.6930	0.6925	0.0005	0.0045
	0.9908	0.9925	-0.0017	0.0045
590 nm	0.0000	0.0000	0.0000	0.0045
	0.2443	0.2452	-0.0009	0.0045
	0.5530	0.5544	-0.0014	0.0045
	0.7196	0.7195	0.0001	0.0045
	1.0301	1.0316	-0.0015	0.0045
635 nm	0.0000	0.0000	0.0000	0.0045
	0.2646	0.2651	-0.0005	0.0045
	0.5370	0.5394	-0.0024	0.0045
	0.6862	0.6872	-0.0010	0.0045
	0.9822	0.9855	-0.0033	0.0045

The End of Certificate**บริษัท ชายนีเมท จำกัด (SCIMET CO., LTD.)**


1194 Soi Wachirathamsathit 57, Bangchak, Phrakhanong, Bangkok 10260 Thailand

Email: scimet2022@gmail.com, Tel: 02 460 9239



FC07-03: 30 MAY 2023

ผู้ตรวจการฝ่ายควบคุมคุณภาพ



Refer to Certificate No.: C07240032

Page: 1 of 3

Statements of conformity:

This conformity certificate documents the validity of the following statements of conformity based on the measurement results of corresponding calibration certificate:

The error of temperature determined during calibration are under given measurement and environmental conditions and considering the expanded measurement uncertainty (coverage probability 95%) within the specification. The given measurement uncertainty already includes other all effects by according to the standard method, ASTM E 275-08 and ASTM E 387-04. Therefore, those parameters have not been assessed separately.

Tolerance and Decision rules:

Assessment of the conformity of the measurement device are done based on direct comparison of the relevant measurement results with the tolerances and decision rule are prescribed by the customer.

- Decision rule :** ☐ Choice A Binary Statement for Simple Acceptance Rule ($w = 0$), Specific Risk $< 50\%$ PFA.
- ☒ Choice B Non-binary statement with guard band ($w = 1 U$), Pass or Fail Specific Risk $< 2.5\%$ PFA and Condition Pass or Condition Fail Specific Risk $< 50\%$ PFA.
- ☐ Choice C Customer defined, Customers may define arbitrary multiple of r to have applied as guard band ($w = r U$).
- ; PFA – Probability of False Accept



(Mr. [Redacted] am)


Authorized signatory

บริษัท ชายนันเมท จำกัด (SCIMET CO., LTD.)

1194 Sol Wachirathamsathit 57, Bangchak, Phrakhanong, Bangkok 10260 Thailand
Email: scimet2022@gmail.com, Tel: 02 460 9239



รับรองสำเนาถูกต้อง
FC07-03: 30 MAY 2023
ผู้จัดทำ: [Redacted]



Refer to Certificate No.: C07240032

Page: 2 of 3

Without Adjustment**Wavelength Accuracy (nm), The spectral bandwidth of Std at 1.5 nm and UUC at 1.5 nm**


Unit Under Calibration	Correction	Guard Band (w)	Tolerance (\pm)	Conformity
220.0	-0.27	0.14	1.0	Pass
241.8	-0.25	0.16	1.0	Pass
287.6	-0.04	0.14	1.0	Pass
333.7	0.07	0.19	1.0	Pass
360.1	0.35	0.14	1.0	Pass
417.0	0.59	0.14	1.0	Pass
472.3	0.20	0.14	1.0	Pass
513.4	0.07	0.14	1.0	Pass
528.9	-0.02	0.14	1.0	Pass
537.1	0.08	0.14	1.0	Pass
642.3	-0.72	0.16	1.0	Pass
741.3	-0.58	0.14	1.0	Pass
749.1	-0.55	0.14	1.0	Pass
807.4	-0.37	0.14	1.0	Pass
879.0	0.28	0.14	1.0	Pass

Photometric Accuracy (Absorbance)

Wavelength	Unit Under Calibration	Correction	Guard Band (w)	Tolerance (\pm)	Conformity
235 nm	0.0000	0.0000	0.0080	0.020	Pass
	0.7273	0.0020	0.0080	0.020	Pass
257 nm	-0.0003	0.0003	0.0080	0.020	Pass
	0.8457	0.0040	0.0080	0.020	Pass
313 nm	0.0004	-0.0004	0.0080	0.020	Pass
	0.2810	0.0023	0.0080	0.020	Pass
350 nm	0.0001	-0.0001	0.0080	0.020	Pass
	0.6259	0.0040	0.0080	0.020	Pass

บริษัท ชายนีเมท จำกัด (SCIMET CO., LTD.)1194 Soi Wachirathamsathit 57, Bangchak, Phrakhanong, Bangkok 10260 Thailand
Email: scimet2022@gmail.com, Tel: 02 460 9239

FC07-03: 30 MAY 2023



Refer to Certificate No.: C07240032

Page: 3 of 3

Without Adjustment

Photometric Accuracy (Absorbance)

Wavelength	Unit Under Calibration	Correction	Guard Band (w)	Tolerance (\pm)	Conformity
420 nm	0.0000	0.0000	0.0045	0.015	Pass
	0.2386	-0.0013	0.0045	0.015	Pass
	0.5637	-0.0020	0.0045	0.015	Pass
	0.7382	0.0010	0.0045	0.015	Pass
	1.0542	0.0008	0.0045	0.015	Pass
440 nm	0.0000	0.0000	0.0045	0.015	Pass
	0.2354	-0.0019	0.0045	0.015	Pass
	0.5539	-0.0026	0.0045	0.015	Pass
	0.7222	0.0008	0.0045	0.015	Pass
	1.0343	-0.0019	0.0045	0.015	Pass
465 nm	0.0000	0.0000	0.0045	0.015	Pass
	0.2143	-0.0017	0.0045	0.015	Pass
	0.5059	-0.0023	0.0045	0.015	Pass
	0.6729	0.0006	0.0045	0.015	Pass
	0.9638	-0.0023	0.0045	0.015	Pass
546.1 nm	0.0000	0.0000	0.0045	0.015	Pass
	0.2213	-0.0012	0.0045	0.015	Pass
	0.5196	-0.0020	0.0045	0.015	Pass
	0.6925	0.0005	0.0045	0.015	Pass
	0.9925	-0.0017	0.0045	0.015	Pass
590 nm	0.0000	0.0000	0.0045	0.015	Pass
	0.2452	-0.0009	0.0045	0.015	Pass
	0.5544	-0.0014	0.0045	0.015	Pass
	0.7195	0.0001	0.0045	0.015	Pass
	1.0316	-0.0015	0.0045	0.015	Pass
635 nm	0.0000	0.0000	0.0045	0.015	Pass
	0.2651	-0.0005	0.0045	0.015	Pass
	0.5394	-0.0024	0.0045	0.015	Pass
	0.6872	-0.0010	0.0045	0.015	Pass
	0.9855	-0.0033	0.0045	0.015	Pass

The validity of the statements of conformity cannot be guaranteed for different places of use, environmental conditions or improper use.


The End of Statements of Conformity

บริษัท ชายนิเมท จำกัด (SCIMET CO., LTD.)

1194 Soi Wachirathamsathit 57, Bangchak, Phrakhanong, Bangkok 10260 Thailand

Email: scimet2022@gmail.com, Tel: 02 460 9239

วันที่ 11/05/2022
สถานที่ วัดพระธาตุทอง



ใบตรวจสอบสภาพเครื่อง Spectrophotometer

เลขที่ใบงาน: KSMT2400444

ชนิดเครื่องมือ: SPECTROPHOTOMETER

รุ่น: CARY 60UV-VIS

หมายเลขเครื่อง: MY17490026

ตรวจสอบ (รับ)		รายการตรวจเช็ค	ตรวจสอบ (ส่ง)		หมายเหตุ
04 Mar 2024			04 Mar 2024		
ปกติ	ไม่ปกติ		ปกติ	ไม่ปกติ	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	1. ความสมบูรณ์เครื่อง	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	2. ความสะอาด (ช่องใส่ตัวอย่าง, ภายใน-นอกเครื่อง)	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	3. สวิตช์ ปิด – เปิด เครื่อง (On-Off Swicth)	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	4. ปุ่มกด (Keypad)	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	5. หน้าจอ (Display, Screen Contrast)	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	6. ตัวหมุนเลือกความยาวคลื่น (Wavelength Control)	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	7. ความยาวคลื่น (Wavelength Check)	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	8. แหล่งกำเนิดแสง (UV < 3,000 hour)	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	9. แหล่งกำเนิดแสง (Visible < 5,000 hour)	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input type="checkbox"/>	<input type="checkbox"/>	10. ช่องวัดหลายตัวอย่าง (Carousel Module)	<input type="checkbox"/>	<input type="checkbox"/>	-

เพิ่มเติม/ข้อแนะนำ :

Mr. Dumrong Boonsopon

Service Engineer

บริษัท ชายนัมเมก จำกัด (SCIMET CO., LTD.)

1194 Soi Wachirathamsathit 57, Bangchak, Phrakhanong, Bangkok 10260 Thailand
Email: scimet2022@gmail.com, Tel: 02 460 9239



F107-01: 08 MAR 2023

CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhprachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech.cal@yahoo.com, calibratech.cal@hotmail.com



Certificate of Calibration

Certificate No. : 67-400054-2

Page : 1 of 2

Submitted by : Envilab Co., Ltd.

540,540/1 Soi Bangkhae7, Bangkhae, Bangkok 10160

Equipment : Autoclave

Manufacturer : Tomy

Model : SX-500

Range : N/A °C

Resolution 1 °C

Serial No. : 55133094

ID No. : N/A

Environment : On site calibration was carried out at the Laboratory, Envilab Co., Ltd.

Ambient Temperature : (30.0 to 31.0) °C

Relative Humidity : (50 to 55) %

Line Voltage : (224.0 to 225.0) V

Date of Received : 01 February 2024

Date of Calibration : 01 February 2024

Date of Issue : 03 February 2024

Calibrated by : Perimon Chanpu

Calibration Method : This instrument was calibrated by In-house method CAL-M4007 based on BS 2646 Part 1 : 2021

The temperature scale used was based on ITS-90

Reference Standard Instruments : This certification is traceable to the International System of Units

Standard Temperature Data Logger with RTD pt 100

ID No.	Cert. No.	Due Date	Traceability
400039	66-400707-1	27 Jun 2024	National Institute of Metrology Thailand (NIMT)
400040	66-400707-2	27 Jun 2024	National Institute of Metrology Thailand (NIMT)
400041	66-400707-3	27 Jun 2024	National Institute of Metrology Thailand (NIMT)

Approved by

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



รับรองสำเนาถูกต้อง
Envilab Co., Ltd.



CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhprachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech.cal@yahoo.com, calibratech.cal@hotmail.com

Certificate of Calibration


Certificate No. 67-400054-2

Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Function : Temperature measurement

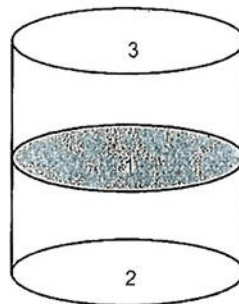

Front

Test Point (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Temperature (°C) @ Sensor No.			Uncertainty (± °C)	Measured Uniformity (°C)	Measured Stability (°C)	Sterilizing Time (minute)	Pressure Gauge Reading (MPa)
			1	2	3					
121	121	121	121.4	121.4	121.4	1.0	1.0	0.5	15	0.11

Remark

1. UUC : Unit Under Calibration
2. Pressure Gauge reading are out of accreditation's scope.

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

- oOo -



EnviLab Co., Ltd.

รับรองสำเนาถูกต้อง
ผู้จัดการฝ่ายควบคุมคุณภาพ



CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhaprachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech_cal@yahoo.com, calibratech_cal@hotmail.com



NSC-TISI-TIS17025
CALIBRATION 0030

Certificate of Calibration

Certificate No. : 67-400101-1

Page : 1 of 2

Submitted by : Envilab Co., Ltd.

540, 540/1 Soi Bangkhuae 7, Bangkhuae, Bangkok 10160

Equipment : Temperature controlled enclosure (Incubator)

Manufacturer : Memmert

Model : IF 110

Range : N/A °C

Resolution : 0.1 °C

Serial No. : D419.0525

ID No. : ELABINCUBATOR1

Environment : On site calibration was carried out at the Laboratory, Envilab Co., Ltd.

Ambient Temperature : (23.0 to 24.0) °C

Relative Humidity : (50 to 55) %

Line Voltage : (223.0 TO 225.0)V

Date of Received : 20 February 2024

Date of Calibration : 20 February 2024

Date of Issue : 22 February 2024

Calibrated by : Kittisak Kokaeo

Calibration Method : CAL-M4004, TLAS G-20

The temperature scale used was based on ITS-90

Reference Standard Instruments : This certification is traceable to the International System of Units

Standard Digital Thermometer with RTD Probe

<u>ID No.</u>	<u>Cert. No.</u>	<u>Due Date</u>	<u>Traceability</u>
400046 & 400042	67-400047-1	25 Jul 2024	National Institute of Metrology Thailand (NIMT)

Approved by

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co., Ltd.



Envilab Co.,Ltd.

ผู้จัดการฝ่ายควบคุมคุณภาพ



Certificate of Calibration

Certificate No. : 67-400101-1


Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Function : Temperature measurement

This instrument was setting air ventilation at position 0 (close)

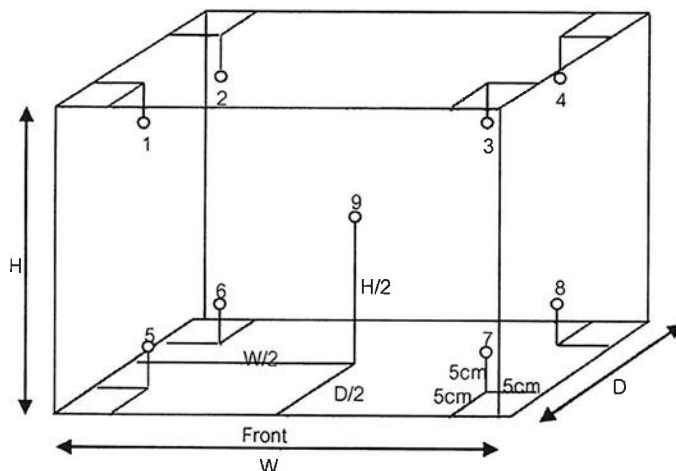

Inside of Chamber

W = 0.56 m

D = 0.48 m

H = 0.40 m

Capacity = 0.11 m³

Test Point (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Temperature (°C) @ Sensor No.									Uncertainty (± °C)
			1	2	3	4	5	6	7	8	9	
35.0	35.0	35.0	35.00	35.10	35.16	35.14	35.15	35.14	35.03	35.00	35.12	0.30
37.0	37.0	37.0	37.01	37.11	37.17	37.15	37.16	37.15	37.04	37.01	37.13	0.30

Test Point (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Uniformity (°C)	Measured Stability (°C)	Overall Variation (°C)
35.0	35.0	35.0	0.1	0.0	0.2
37.0	37.0	37.0	0.1	0.0	0.2

Remark The uncertainty is not combine uniformity of the air chamber

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

- o0o -



Envilab Co.,Ltd.

ผู้จัดการฝ่ายควบคุมคุณภาพ

CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhprachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech-cal@yahoo.com, calibratech-cal@hotmail.com



NSC-TISI-TIS17025
CALIBRATION 0030

Certificate of Calibration

Certificate No. : 66-400477-1

Page : 1 of 2

Submitted by : Envilab Co.,Ltd.

540 . 540/1 Soi Bangkhac 7, Bangkhac ,Bangkok 10160

Equipment : Water Bath

Manufacturer : LAUDA

Model : A 24

Range : N/A °C

Resolution : 0.1 °C

Serial No. : CN21001882

ID No. : ELABWBALPHA241

Environment : On site calibration was carried out at the Laboratory,ENVILAB CO.LTD

Ambient Temperature : (22.5 to 23.0) °C

Relative Humidity : (40 to 45) %

Line Voltage : (228.0 to 230.1)V

Date of Received : 25 August 2023

Date of Calibration : 25 August 2023

Date of Issue : 25 August 2023

Calibrated by : Permpon Chanpu

Calibration Method : This instrument was calibrated by In-house method CAL-M4006 based on ASTM E715-80
The temperature scale used was based on ITS-90

Reference Standard Instruments : This certification is traceable to the International System of Units
Standard Digital Thermometer with RTD probe

<u>ID No.</u>	<u>Cert. No.</u>	<u>Due Date</u>	<u>Traceability</u>
400046 & 400024	66-400184-2	06 Oct 2023	National Institute of Metrology Thailand (NIMT)

Approve

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Envilab Co.,Ltd.

ผู้ตรวจการฝ่ายควบคุมคุณภาพ



Certificate of Calibration


Certificate No. : 66-400477-1

Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Function : Temperature measurement

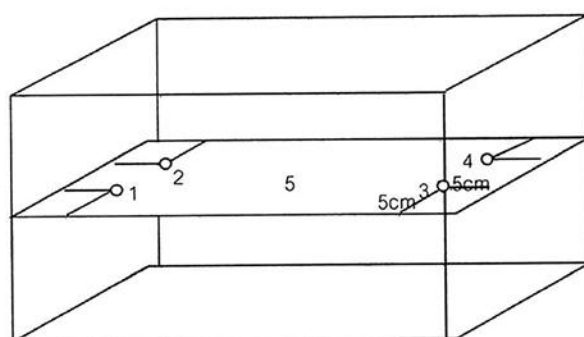

Front

Test Point (° C)	Setting Temperature (° C)	Indicating Temperature (° C)	Measured Temperature (° C) @ Sensor					Uncertainty (± ° C)	Measured Uniformity (° C)	Measured Stability (° C)
			No.							
			1	2	3	4	5			
44.5	44.5	44.5	44.52	44.50	44.50	44.50	44.50	0.18	0.06	0.01

Remark The uncertainty is not combine uniformity of the water bath


This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

- o0o -




Envilab Co.,Ltd.

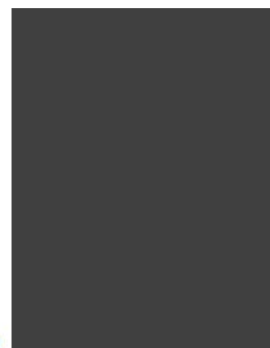

รับรองสำเนา
ผู้จัดการฝ่ายควบคุมคุณภาพ





ภาคผนวก ค-3

เอกสารขึ้นทะเบียนห้องปฏิบัติการ



ใบรับรองเลขที่ 20T218/1196

ใบรับรองห้องปฏิบัติการ

อาศัยอำนาจตามความในพระราชบัญญัติการมาตรฐานแห่งชาติ พ.ศ. ๒๕๕๑

เลขาธิการสำนักงานมาตรฐานผลิตภัณฑ์อุตสาหกรรม

ออกใบรับรองฉบับนี้ให้

บริษัท เอ็นไวแล็บ จำกัด

มีห้องปฏิบัติการตั้งอยู่เลขที่

540, 540/1 ซอยบางแค 7 แขวงบางแค เขตบางแค กรุงเทพมหานคร

ได้รับการรับรองความสามารถห้องปฏิบัติการทดสอบ

ตามมาตรฐานเลขที่ มอก. 17025-2561 (ISO/IEC 17025 : 2017)

ข้อกำหนดทั่วไปว่าด้วยความสามารถห้องปฏิบัติการทดสอบและสอบเทียบ

หมายเลขการรับรองที่ ทดสอบ ๐๕๒๖

โดยมีสาขาการรับรองตามรายละเอียดแนบท้ายใบรับรอง

ตั้งแต่วันที่ ๒๓ พฤศจิกายน พ.ศ. ๒๕๖๓

ถึง วันที่ ๒๒ พฤศจิกายน พ.ศ. ๒๕๖๖

ออกให้ ณ วันที่ - ๙ ธ.ค. ๒๕๖๓

(ใน [redacted] น์)

รอง [redacted] แทน

เลขาธิการสำนักงานมาตรฐานผลิตภัณฑ์อุตสาหกรรม



กระทรวงอุตสาหกรรม สำนักงานมาตรฐานผลิตภัณฑ์อุตสาหกรรม

ที่ อก ๐๓๑๐(๑)/ ๑๓๔๙๖



กรมโรงงานอุตสาหกรรม
ถนนพระรามที่ ๖ แขวงทุ่งพญาไท
เขตราชเทวี กรุงเทพฯ ๑๐๕๐๐

๒๐ กันยายน ๒๕๖๖

เรื่อง ต่ออายุหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน

เรียน กรรมการผู้จัดการ บริษัท เอ็นไวแล็บ จำกัด

อ้างถึง คำขอขึ้นทะเบียน/ต่ออายุ/เปลี่ยนแปลงบุคลากร และชนิดสารมลพิษของห้องปฏิบัติการวิเคราะห์เอกชน
ลงวันที่ ๑๐ กรกฎาคม ๒๕๖๖

- สิ่งที่ส่งมาด้วย ๑. รายชื่อผู้ควบคุมดูแลห้องปฏิบัติการวิเคราะห์ จำนวน ๑ แผ่น
๒. รายชื่อเจ้าหน้าที่ประจำห้องปฏิบัติการวิเคราะห์ จำนวน ๒ แผ่น
๓. ขอบข่ายสารมลพิษที่ได้รับขึ้นทะเบียนจากกรมโรงงานอุตสาหกรรม จำนวน ๙ แผ่น

ตามหนังสือที่อ้างถึง บริษัท เอ็นไวแล็บ จำกัด ขอต่ออายุหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน เลขทะเบียน ว-๑๑๘ สถานที่ตั้งเลขที่ ๕๔๐, ๕๔๐/๑ ซอยบางแค ๗ แขวงบางแค เขตบางแค กรุงเทพมหานคร ต่อกรมโรงงานอุตสาหกรรม นั้น

กรมโรงงานอุตสาหกรรมพิจารณาแล้ว ให้บริษัท เอ็นไวแล็บ จำกัด ต่ออายุหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน โดยมีองค์ประกอบดังนี้

- ก. ผู้ควบคุมดูแลห้องปฏิบัติการวิเคราะห์ จำนวน ๓ ราย ตามสิ่งที่ส่งมาด้วย ๑
ข. เจ้าหน้าที่ประจำห้องปฏิบัติการวิเคราะห์ ๔๗ ราย ตามสิ่งที่ส่งมาด้วย ๒
ค. ขอบข่ายสารมลพิษที่ได้รับขึ้นทะเบียนให้วิเคราะห์ในน้ำเสีย น้ำใต้ดิน อากาศเสีย สิ่งปฏิกูลหรือวัสดุที่ไม่ใช่แล้ว และดิน ตามสิ่งที่ส่งมาด้วย ๓

หนังสือฉบับนี้จะหมดอายุในวันที่ ๑๔ กรกฎาคม ๒๕๖๙ หากประสงค์จะต่ออายุหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน ให้ยื่นคำขอต่ออายุพร้อมเอกสารประกอบคำขอต่อกรมโรงงานอุตสาหกรรม ภายใน ๓๐ วัน ก่อนวันสิ้นอายุของหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน ทั้งนี้ สามารถยื่นคำขอผ่านระบบอิเล็กทรอนิกส์ได้ที่หน้าเว็บไซต์กรมโรงงานอุตสาหกรรม

จึงเรียนมาเพื่อทราบ

ขอแสดงความนับถือ



ผู้อำนวยการกองงานและทะเบียนมลพิษโรงงาน
ปฏิบัติราชการแทนอธิบดีกรมโรงงานอุตสาหกรรม

กองวิจัยและเตือนภัยมลพิษโรงงาน

กลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษและทะเบียน

โทร. ๐ ๒๔๓๐ ๖๓๑๒ ต่อ ๒๑๐๓-๕

โทรสาร ๐ ๒๔๓๐ ๖๓๑๒ ต่อ ๒๑๔๙

ไปรษณีย์อิเล็กทรอนิกส์ saraban@diw.mail.go.th



“อุตสาหกรรมก้าวไกล ประเทศไทยก้าวหน้า ร่วมกันพัฒนา อุตสาหกรรมสีเขียว”



เอกสารแนบท้ายหนังสือรับต่ออายุขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน

บริษัท เอ็นไวแล็บ จำกัด

เลขทะเบียน ว-๑๑๘

ที่ อก ๐๓๑๐(๑)/ ๑ ๓ ๔ ๕ ๖

ลงวันที่ ๒๐ กันยายน ๒๕๖๖

ก. ผู้ควบคุมดูแลห้องปฏิบัติการวิเคราะห์ จำนวน ๓ ราย

๑) น

๒) น

๓) น

วิมล



เอกสารแนบท้ายหนังสือรับต่ออายุขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน

บริษัท เอ็นไวแล็บ จำกัด

เลขทะเบียน ว-๑๑๘

ที่ อก ๐๓๑๐(๑)/ ๑ ๓ ๔ ๕ ๖

ลงวันที่ ๒๐ กันยายน ๒๕๖๖

ข. เจ้าหน้าที่ประจำห้องปฏิบัติการวิเคราะห์ จำนวน ๔๗ ราย

๑) น

๒) น

๓) น

๔) น

๕) น

๖) น

๗) น

๘) น

๙) น

๑๐) น

๑๑) น

๑๒) น

๑๓) น

๑๔) น

๑๕) น

๑๖) น

๑๗) น

๑๘) น

๑๙) น

๒๐) น

๒๑) น

๒๒) น

๒๓) น

๒๔) น

๒๕) น

๒๖) น

๒๗) น

๒๘) น

๒๙) น

๓๐) น

๓๑) น

๓๒) น

๓๓) น

๓๔) น

๓๕) น

๓๖) น

๓๗) นางสาวปิยธิดา...

๓๗) นาง
๓๘) นาง
๓๙) นาง
๔๐) นาง
๔๑) นาง
๔๒) นาง
๔๓) นาง
๔๔) นาง
๔๕) นาง
๔๖) นาง
๔๗) นาง



เอกสารแนบท้ายหนังสือรับต่ออายุขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน

บริษัท เอ็นไวแล็บ จำกัด

เลขทะเบียน ว-๑๑๘

ที่ อก ๐๓๑๐(๑)/ ๑ ๓ ๔ ๕ ๖

ลงวันที่ ๒๐ กันยายน ๒๕๖๖

ค. ขอบข่ายสารมลพิษที่ได้รับขึ้นทะเบียนจากกรมโรงงานอุตสาหกรรม จำนวน ๙๙ รายการ

น้ำเสีย จำนวน 23 รายการ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
1	Arsenic	1) Digestion, Hydride Generation/Atomic Absorption Spectrometric Method ^[3] 2) Digestion, Inductively Coupled Plasma Method ^[3]
2	Barium	Digestion, Inductively Coupled Plasma Method ^[3]
3	Biochemical Oxygen Demand	1) 5-Day BOD Test, Azide Modification Method ^[3] 2) 5-Day BOD Test, Membrane Electrode Method ^[3]
4	Cadmium	1) Digestion, Direct Air-Acetylene Flame Method ^[3] 2) Digestion, Inductively Coupled Plasma Method ^[3]
5	Chemical Oxygen Demand	Closed Reflux, Titrimetric Method ^[3]
6	Color	ADMI Weighted-Ordinate Spectrophotometric Method ^[3]
7	Copper	1) Digestion, Direct Air-Acetylene Flame Method ^[3] 2) Digestion, Inductively Coupled Plasma Method ^[3]
8	Free Chlorine	Iodometric Method ^[3]
9	Hexavalent Chromium	Colorimetric Method ^[3]
10	Lead	1) Digestion, Direct Air-Acetylene Flame Method ^[3] 2) Digestion, Inductively Coupled Plasma Method ^[3]
11	Manganese	Digestion, Inductively Coupled Plasma Method ^[3]
12	Mercury	Digestion, Cold-Vapor Atomic Absorption Spectrometric Method ^[3]
13	Nickel	Digestion, Inductively Coupled Plasma Method ^[3]
14	Oil & Grease	Liquid-Liquid, Partition-Gravimetric Method ^[3]
15	pH	Electrometric Method ^[3]
16	Selenium	1) Digestion, Hydride Generation/Atomic Absorption Spectrometric Method ^[3] 2) Digestion, Inductively Coupled Plasma Method ^[3]
17	Sulfide	Iodometric Method ^[3]
18	Temperature	Laboratory and Field Methods ^[3]
19	Total Dissolved Solids	

dahl Nitrogen ...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
20	Total Kjeldahl Nitrogen	1) Macro-Kjeldahl Method ^[3] 2) Semi-Micro-Kjeldahl Method ^[3]
21	Total Suspended Solids	Dried at 103-105 °C ^[3]
22	Trivalent Chromium	Digestion, Inductively Coupled Plasma Method; Colorimetric Method; Calculation ^[3]
23	Zinc	1) Digestion, Direct Air-Acetylene Flame Method ^[3] 2) Digestion, Inductively Coupled Plasma Method ^[3]

น้ำใต้ดิน จำนวน 17 รายการ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
1	Antimony	Digestion, Inductively Coupled Plasma Method ^[3]
2	Arsenic	1) Digestion, Hydride Generation/Atomic Absorption Spectrometric Method ^[3] 2) Digestion, Inductively Coupled Plasma Method ^[3]
3	Barium	Digestion, Inductively Coupled Plasma Method ^[3]
4	Beryllium	Digestion, Inductively Coupled Plasma Method ^[3]
5	Cadmium	1) Digestion, Direct Air-Acetylene Flame Method ^[3] 2) Digestion, Inductively Coupled Plasma Method ^[3]
6	Chromium	Digestion, Inductively Coupled Plasma Method ^[3]
7	Chromium (III)	Digestion, Inductively Coupled Plasma Method; Colorimetric Method; Calculation ^[3]
8	Chromium (VI)	Colorimetric Method ^[3]
9	Lead	1) Digestion, Direct Air-Acetylene Flame Method ^[3] 2) Digestion, Inductively Coupled Plasma Method ^[3]
10	Manganese	Digestion, Inductively Coupled Plasma Method ^[3]
11	Mercury	Digestion, Cold-Vapor Atomic Absorption Spectrometric Method ^[3]
12	Nickel	Digestion, Inductively Coupled Plasma Method ^[3]
13	pH	Electrometric Method ^[3]
14	Selenium	1) Digestion, Hydride Generation/Atomic Absorption Spectrometric Method ^[3] 2) Digestion, Inductively Coupled Plasma Method ^[3]
15	Silver	Digestion, Inductively Coupled Plasma Method ^[3]

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
16	Vanadium	Digestion, Inductively Coupled Plasma Method ^[3]
17	Zinc	1) Digestion, Direct Air-Acetylene Flame Method ^[3] 2) Digestion, Inductively Coupled Plasma Method ^[3]

อากาศเสีย (ปล่องระบาย) จำนวน 24 รายการ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
1	Antimony	Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method ^[4]
2	Arsenic	Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method ^[4]
3	Beryllium	Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method ^[4]
4	Cadmium	Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method ^[4]
5	Carbon monoxide	Instrumental Analyzer Method ^[4]
6	Chromium	Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method ^[4]
7	Cobalt	Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method ^[4]
8	Copper	Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method ^[4]
9	Cresol	Adsorption Sampling, Gas Chromatographic Method ^[4]
10	Dioxins/Furans	Isokinetic Sampling, Analysis by ISO/IEC 17025 Accredited Laboratory or Analysis by Department of Industrial Works Registered Laboratory (Dioxins/Furans Analysis Approved) ^[4]
11	Hydrogen Sulfide	Absorption Sampling, Iodometric Method ^[4]
12	Lead	Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method ^[4]
13	Manganese	Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method ^[4]
14	Mercury	Isokinetic Sampling, Digestion, Cold-Vapor Atomic

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
15	Nickel	Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method ^[4]
16	Opacity	Ringelmann's Method ^[2]
17	Oxides of Nitrogen	1) Absorption Sampling, Phenoldisulfonic acid Method ^[4] 2) Instrumental Analyzer Method ^[4]
18	Selenium	Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method ^[4]
19	Sulfur dioxide	1) Absorption Sampling, Barium-Thorin Titrimetric Method ^[4] 2) Instrumental Analyzer Method ^[4]
20	Sulfuric acid	Isokinetic Sampling, Barium-Thorin Titrimetric Method ^[4]
21	Tin	Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method ^[4]
22	Total Suspended Particulate	Isokinetic Sampling, Gravimetric Method ^[4]
23	Vanadium	Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method ^[4]
24	Xylene	Adsorption Sampling, Gas Chromatographic Method ^[4]

สิ่งปลูกสร้างวัสดุที่ไม่ใช่แล้ว จำนวน 19 รายการ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
1	Antimony	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[1,5,9] 2) Digestion, Inductively Coupled Plasma Method ^[6,9]
2	Arsenic	1) Waste Extraction, Digestion, Hydride Generation/Atomic Absorption Spectrometric Method ^[1,5,11] 2) Digestion, Hydride Generation/Atomic Absorption Spectrometric Method ^[6,11]
3	Barium	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[1,5,9] 2) Digestion, Inductively Coupled Plasma Method ^[6,9]
4	Beryllium	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[6,9]

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
5	Cadmium	1) Waste Extraction, Digestion, Flame Atomic Absorption Spectrometric Method ^[1,5,10] 2) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[1,5,9] 3) Digestion, Flame Atomic Absorption Spectrometric Method ^[6,10] 4) Digestion, Inductively Coupled Plasma Method ^[6,9]
6	Chromium	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[1,5,9] 2) Digestion, Inductively Coupled Plasma Method ^[6,9]
7	Chromium (III)	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method; Waste Extraction, Colorimetric Method; Calculation ^[1,5,8,12] 2) Digestion, Inductively Coupled Plasma Method; Alkaline Digestion, Colorimetric Method; Calculation ^[6,7,8,12]
8	Chromium (VI)	1) Waste Extraction, Colorimetric Method ^[1,12] 2) Alkaline Digestion, Colorimetric Method ^[8,12]
9	Cobalt	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[1,5,9] 2) Digestion, Inductively Coupled Plasma Method ^[6,9]
10	Copper	1) Waste Extraction, Digestion, Flame Atomic Absorption Spectrometric Method ^[1,5,10] 2) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[1,5,9] 3) Digestion, Flame Atomic Absorption Spectrometric Method ^[6,10] 4) Digestion, Inductively Coupled Plasma Method ^[6,9]
11	Lead	1) Waste Extraction, Digestion, Flame Atomic Absorption Spectrometric Method ^[1,5,10] 2) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[1,5,9] 3) Digestion, Flame Atomic Absorption Spectrometric Method ^[6,9]



12 Mercury ...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
12	Mercury	1) Waste Extraction, Digestion, Cold-Vapor Atomic Absorption Spectrometric Method ^[1,5,13] 2) Digestion, Cold-Vapor Atomic Absorption Spectrometric Method ^[14]
13	Molybdenum	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[1,5,9] 2) Digestion, Inductively Coupled Plasma Method ^[6,9]
14	Nickel	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[1,5,9] 2) Digestion, Inductively Coupled Plasma Method ^[6,9]
15	Selenium	1) Waste Extraction, Digestion, Hydride Generation/Atomic Absorption Spectrometric Method ^[1,5,15] 2) Digestion, Hydride Generation/Atomic Absorption Spectrometric Method ^[6,15]
16	Silver	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[1,5,9] 2) Digestion, Inductively Coupled Plasma Method ^[6,9]
17	Thallium	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[1,5,9] 2) Digestion, Inductively Coupled Plasma Method ^[6,9]
18	Vanadium	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[1,5,9] 2) Digestion, Inductively Coupled Plasma Method ^[6,9]
19	Zinc	1) Waste Extraction, Digestion, Flame Atomic Absorption Spectrometric Method ^[1,5,10] 2) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[1,5,9] 3) Digestion, Flame Atomic Absorption Spectrometric Method ^[6,10] 4) Digestion, Inductively Coupled Plasma Method ^[6,9]

ดิน จำนวน 16 รายการ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
1	Antimony	Digestion, Inductively Coupled Plasma Method ^[6,7,9]
2	Arsenic	1) Digestion, Hydride Generation/Atomic Absorption Spectrometric Method ^[6,7,11] 2) Digestion, Inductively Coupled Plasma Method ^[6,7,9]
3	Barium	Digestion, Inductively Coupled Plasma Method ^[6,7,9]
4	Beryllium	Digestion, Inductively Coupled Plasma Method ^[6,7,9]
5	Cadmium	1) Digestion, Flame Atomic Absorption Spectrometric Method ^[6,7,10] 2) Digestion, Inductively Coupled Plasma Method ^[6,7,9]
6	Chromium	Digestion, Inductively Coupled Plasma Method ^[6,7,9]
7	Chromium (III)	Digestion, Inductively Coupled Plasma Method; Alkaline Digestion, Colorimetric Method; Calculation ^[6,7,8,9,12]
8	Chromium (VI)	Alkaline Digestion, Colorimetric Method ^[8,12]
9	Lead	1) Digestion, Flame Atomic Absorption Spectrometric Method ^[6,7,10] 2) Digestion, Inductively Coupled Plasma Method ^[6,7,9]
10	Mercury	Digestion, Cold-Vapor Atomic Absorption Spectrometric Method ^[14]
11	Manganese	Digestion, Inductively Coupled Plasma Method ^[6,7,9]
12	Nickel	Digestion, Inductively Coupled Plasma Method ^[6,7,9]
13	Selenium	1) Digestion, Hydride Generation/Atomic Absorption Spectrometric Method ^[6,7,15] 2) Digestion, Inductively Coupled Plasma Method ^[6,7,9]
16	Silver	Digestion, Inductively Coupled Plasma Method ^[6,7,9]
18	Vanadium	Digestion, Inductively Coupled Plasma Method ^[6,7,9]
19	Zinc	1) Digestion, Flame Atomic Absorption Spectrometric Method ^[6,7,10] 2) Digestion, Inductively Coupled Plasma Method ^[6,7,9]

เอกสารอ้างอิง

1. กระทรวงอุตสาหกรรม. ประกาศกระทรวงอุตสาหกรรม, พ.ศ. 2548. เรื่อง การกำจัดสิ่งปฏิภูลหรือวัสดุที่ไม่ใช้แล้ว.ราชกิจจานุเบกษา. 25 มกราคม 2549. เล่มที่ 123 ตอนพิเศษ 11ง.
2. กระทรวงอุตสาหกรรม. ประกาศกระทรวงอุตสาหกรรม, พ.ศ. 2549. เรื่อง กำหนดค่าปริมาณเขม่าควันที่เจือปนในอากาศที่ระบายออกจากปล่องของหม้อน้ำโรงสีข้าวที่ใช้แกลบเป็นเชื้อเพลิง.ราชกิจจานุเบกษา. 4 ธันวาคม 2549. เล่มที่ 123 ตอนพิเศษ 125ง.
3. APHA, AWWA, WEF. **Standard Methods for the Examination of Water and Wastewater**. 23rd ed. Washington, DC: APHA, 2017.
4. United States Environmental Protection Agency. **Standards of Performance for New Stationary Sources**. 40 CFR 60. Appendix A, 2022.
5. United States Environmental Protection Agency. **Test Methods for Evaluation Solid Waste Physical/Chemical Methods. SW-846**, 1997.
6. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Acid Digestion of Sediment, Sludges, and Soils, SW-846 Method 3050B**, 1996.
7. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Microwave Assisted Acid Digestion of Sediments, Sludges, and Oils. SW-846 Method 3051A**, 2007.
8. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Alkaline Digestion for Hexavalent Chromium. SW-846 Method 3060A**, 1996.
9. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Inductively Coupled Plasma-Atomic Emission Spectrometry. SW-846 Method 6010D**, 2018.
10. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Flame Atomic Absorption Spectrophotometry. SW-846 Method 7000B**, 2007.
11. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Antimony and Arsenic (Atomic Absorption, Borohydride Reduction). SW-846 Method 7062**, 1994.
12. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Chromium, Hexavalent (Colorimetric). SW-846 Method 7196A**, 1992.
13. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods.  (Cold-Vapor-Technique). SW-846 Method 7470A, 1994.
14. United States...

14. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Mercury in Solid or Semisolid Wastes (Manual Cold-Vapor Technique). SW-846 Method 7471B**, 2007.

15. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Selenium (Atomic Absorption, Borohydride Reduction). SW-846 Method 7742**, 1996





ที่ อก ๐๗๑๔/ ๑๒๓๓

สำนักงานมาตรฐานผลิตภัณฑ์อุตสาหกรรม
ถนนพระรามที่ ๖ แขวงทุ่งพญาไท
เขตราชเทวี กรุงเทพฯ ๑๐๕๐๐

๓๐ พฤศจิกายน ๒๕๖๖

เรื่อง สถานะการรับรองความสามารถห้องปฏิบัติการ

เรียน กรรมการผู้จัดการบริษัท เอ็นไวแล็บ จำกัด

อ้างถึง คำขอต่ออายุการรับรองความสามารถห้องปฏิบัติการทดสอบบริษัท เอ็นไวแล็บ จำกัด ผ่านระบบ e-Accreditation วันที่ ๑ กรกฎาคม ๒๕๖๖ เลขที่คำขอ TEST-๖๖-๓๑๓

ตามที่อ้างถึง ห้องปฏิบัติการทดสอบบริษัท เอ็นไวแล็บ จำกัด ได้ยื่นคำขอต่ออายุการรับรองห้องปฏิบัติการทดสอบ ตามมาตรฐานเลขที่ มอก. 17025-2561 ในระบบ e-Accreditation เลขที่คำขอ TEST-๖๖-๓๑๓ นั้น

สำนักงานมาตรฐานผลิตภัณฑ์อุตสาหกรรม ได้ตรวจสอบแล้วพบว่าห้องปฏิบัติการได้รับการรับรองความสามารถห้องปฏิบัติการตามมาตรฐานเลขที่ มอก. 17025-2561 หมายเลขการรับรองที่ ทดสอบ ๐๕๒๖ ใบรับรองเลขที่ ๒๐T๒๑๘/๑๑๙๖ โดยระบุวันสิ้นอายุการรับรองวันที่ ๒๒ พฤศจิกายน ๒๕๖๖ และต่อมาห้องปฏิบัติการได้ยื่นคำขอต่ออายุการรับรองห้องปฏิบัติการทดสอบ เมื่อวันที่ ๑ กรกฎาคม ๒๕๖๖ ซึ่งตามพระราชบัญญัติการมาตรฐานแห่งชาติ พ.ศ. ๒๕๕๑ มาตรา ๒๙ ให้นำมาตรา ๒๐ ของพระราชบัญญัติการมาตรฐานแห่งชาติ พ.ศ. ๒๕๕๑ มาใช้บังคับแก่ผู้รับใบรับรองโดยอนุโลมซึ่งห้องปฏิบัติการได้ปฏิบัติตาม ดังนั้น จึงถือได้ว่าเป็นผู้รับใบรับรองจนกว่าจะมีคำสั่งไม่อนุญาตให้ต่ออายุใบรับรองจากเลขาธิการสำนักงานมาตรฐานผลิตภัณฑ์อุตสาหกรรม

จึงเรียนมาเพื่อทราบ

ขอแสดงความนับถือ



นักวิชาการมาตรฐานชำนาญการพิเศษ

รักษาราชการแทน

ผู้อำนวยการสำนักงานคณะกรรมการมาตรฐานผลิตภัณฑ์

บริการราชการแทน

เลขาธิการสำนักงานมาตรฐานผลิตภัณฑ์อุตสาหกรรม

สำนักงานคณะกรรมการการมาตรฐานแห่งชาติ

กลุ่มรับรองห้องปฏิบัติการ ๒

โทร ๐ ๒๔๓๐ ๖๘๒๕

โทรสาร ๐ ๒๓๕๔ ๓๑๓๓



ENVILAB CO.,LTD

540, 540/1 Soi Bangkhae 7, Bangkhae, Bangkok 10160, Thailand. Tel. 02-802-3577 Fax. 02-802-3773

E-mail : info@evltesting.com Http ://www.evltesting.com

