

ภาคผนวก ง

---

ใบรับรองการสอบเทียบเครื่องมือ



right solutions.  
right partner.

รายการเครื่องมือที่ใช้ในการวิเคราะห์ / ทดสอบ

Sample Name	Parameter	Equipment Name	ID No.	Calibrated Date	Next Cal	Freq. Calibrate (Months)
Water Lab	Lead	ICP-MS	BKK_EL0026	12-Dec-23	13-Jun-25	18
Water Lab	Lead	Hot Block	BKK_EL0054	22-Sep-23	22-Mar-25	18
Water Lab	Lead	Chamber (Cooling Room)	BKK_EN0167	6-Dec-23	6-Jun-25	18
Water Lab	Cadmium	ICP-MS	BKK_EL0026	12-Dec-23	13-Jun-25	18
Water Lab	Cadmium	Hot Block	BKK_EL0054	22-Sep-23	22-Mar-25	18
Water Lab	Cadmium	Chamber (Cooling Room)	BKK_EN0167	6-Dec-23	6-Jun-25	18
Water Lab	Mercury	Mercury Analyzer	BKK_EL0128	6-Dec-23	6-Dec-24	12
Water Lab	Total Coliform	Autoclave	BKK_ML0037	17-Jul-23	17-Jan-25	18
Water Lab	Total Coliform	Incubator	BKK_ML0010	17-Jul-23	17-Jan-25	18
Water Lab	Total Coliform	Hot Air Oven	BKK_ML0013	23-Apr-24	23-Oct-25	18
Water Lab	Fecal Coliform	Autoclave	BKK_ML0037	17-Jul-23	17-Jan-25	18
Water Lab	Fecal Coliform	Incubator	BKK_ML0010	17-Jul-23	17-Jan-25	18
Water Lab	Fecal Coliform	Hot Air Oven	BKK_ML0013	23-Apr-24	23-Oct-25	18
Water Lab	Fecal Coliform	Water Bath	BKK_ML0056	1-Mar-24	1-Mar-25	12
Water Lab	BOD	DO Meter	BKK_EN0017	16-Nov-23	16-May-25	18
Water Lab	BOD	Incubator	BKK_EN0304	20-Mar-24	20-Mar-25	12
Water Lab	BOD	Burette	BKK_EN0171	27-Feb-24	27-Aug-25	18
Water Lab	COD	Hot Block	BKK_EN0222	22-Apr-24	22-Apr-25	12
Water Lab	COD	Spectrophotometer	BKK_EN0018	13-Sep-24	13-Sep-25	12
Water Lab	Color	Chamber (Cooling Room)	BKK_EN0167	6-Dec-23	6-Jun-25	18
Water Lab	Conductivity	Conductivity meter	BKK_EN0373	25-Dec-23	25-Dec-24	12
Water Lab	Dissolved Oxygen (on site)	DO Meter	CHM_LG0002	19-Jun-24	19-Jun-25	12
Water Lab	Oil & Grease	Electronic Top-Loading Balance	BKK_EN0003	2-Aug-24	2-Aug-25	12
Water Lab	Oil & Grease	Water Bath	BKK_EN0148	4-Jul-23	4-Jan-25	18
Water Lab	pH at 25 °C	pH meter	BKK_EN0342	17-Oct-24	17-Oct-25	12
Water Lab	Phosphate	Discrete analyzer	BKK_EN0037	16-Aug-24	16-Aug-25	12
Water Lab	Settleable Solids	Chamber (Cooling Room)	BKK_EN0167	6-Dec-23	6-Jun-25	18
Water Lab	Sulfide	Burette	BKK_EN0171	27-Feb-24	27-Aug-25	18
Water Lab	Sulfide	Chamber (Cooling Room)	BKK_EN0167	6-Dec-23	6-Jun-25	18
Water Lab	Temperature	pH meter	CHM_LG0001	19-Feb-24	19-Feb-25	12
Water Lab	Total Dissolved Solids 103-105°C	Electronic Top-Loading Balance	BKK_EN0003	2-Aug-24	2-Aug-25	12
Water Lab	Total Dissolved Solids 103-105°C	Oven	BKK_EN0273	14-May-24	14-Nov-25	18
Water Lab	Total Kjeldahl Nitrogen	Digestion Unit	BKK_EN0366	21-Apr-24	21-Apr-25	12
Water Lab	Total Kjeldahl Nitrogen	Discrete analyzer	BKK_EN0037	16-Aug-24	16-Aug-25	12
Water Lab	Total Suspended Solids	Electronic Top-Loading Balance	BKK_EN0003	2-Aug-24	2-Aug-25	12
Water Lab	Total Suspended Solids	Oven	BKK_EN0273	14-May-24	14-Nov-25	18
Water Lab	Total Dissolved Solids 180°C	Electronic Top-Loading Balance	BKK_EN0003	2-Aug-24	2-Aug-25	12
Water Lab	Total Dissolved Solids 180°C	Oven	BKK_EN0273	14-May-24	14-Nov-25	18
Ambient	Nitrogen Dioxide	NO <sub>2</sub> Analyzer	BKK_FS1092	3-Jul-24	3-Jan-25	6
Ambient	Sulfur Dioxide	SO <sub>2</sub> Analyzer	BKK_FS1091	5-Jul-24	5-Jan-25	6
Ambient	Particulate Matter (PM-10)	High Volume	BKK_FS1060	-	-	On site Calibration
Ambient	Particulate Matter (PM-10)	Digital Balance	BKK_EN0403	3-Jun-24	3-Jun-25	12
Ambient	Total Suspended Particulate	High Volume	BKK_FS1056	-	-	On site Calibration
Ambient	Total Suspended Particulate	Digital Balance	BKK_EN0403	3-Jun-24	3-Jun-25	12
Ambient	Total Hydrocarbon	DRYCAL FLOWMETER	BKK_FS1346	29-Jan-24	28-Jan-25	12
Ambient	Total Hydrocarbon	Total Hydrocarbon Analyzer	BKK_FS1068	11-Dec-23	11-Jun-25	18
Ambient	Carbon Monoxide	DRYCAL FLOWMETER	BKK_FS1346	29-Jan-24	28-Jan-25	12
Ambient	Carbon Monoxide	CO Analyzer	BKK_EN0375	5-Aug-24	5-Aug-25	12



## Agilent Technologies

Agilent Technologies (Thailand) Limited  
U CHU LIANG BLDG. 22/F UNIT A,D  
968 RAMA 4 ROAD, SILOM, BANGRAK  
Bangkok 10500 Thailand

Tel. +662 637 6363  
Fax: +662 632 4334  
Email: [ccc-smt@agilent.com](mailto:ccc-smt@agilent.com)  
Website: [www.agilent.com/chem](http://www.agilent.com/chem)

### Customer Contact:

ALS Laboratory Group (Thailand) Co  
Ltd  
Head Office  
104 Phatthanakan 40 Phatthanakan Rd  
Khwaeng Phatthanakan Khet Suan  
TAX ID : 0105540004859  
Chanattagarn.lmchom@alsglobal.com  
27603068

### Invoice To:

ALS Laboratory Group (Thailand) Co  
Ltd  
Head Office  
104 Phatthanakan 40 Phatthanakan Rd  
Khwaeng Phatthanakan Khet Suan

### Delivery Site:

ALS Laboratory Group (Thailand) Co  
Ltd  
Head Office  
104 Phatthanakan 40 Phatthanakan Rd  
Khwaeng Phatthanakan Khet Suan

### Location:

Room  
Bldg  
Lab  
Dept

## SERVICE REPORT

<b>Customer Purchase Order Number:</b>	<b>Customer Number:</b> 70371013
<b>Service Request:</b>	<b>Service Request Date:</b>
<b>Service Order:</b> 6006041263	<b>Service Confirmation:</b> 6905338201

REVIEW BY	Supakwan M.
APPROVED BY	Savitri N.
NEXT CAL. DATE	13/06/2025

### Direct Inquiries to:

Contact Name: Customer Contact Center  
Contact E-mail: [ccc-smt@agilent.com](mailto:ccc-smt@agilent.com)  
Contact Telephone: +662 637 6363  
Contact Fax: +662 632 4334

products | applications | software | services

Learn more about Agilent's Special Offers, Products, Services and our full range of laboratory productivity solutions optimized for your applications and workflows. Visit us at [www.agilent.com/chem](http://www.agilent.com/chem)

Agilent Technologies (Thailand) Limited, Head Office  
U Chu Liang Bldg, 22/F Unit A,D  
968 Rama 4 Road, Silom, Bangrak,  
Bangkok 10500 Thailand  
Tax ID : 0105542068218

Citibank N.A. Bangkok Branch  
399 Interchange 21 Building, Sukhumvit Road, Klongtoey Nau  
Sub-district, Wattana District, Bangkok 10110 Thailand  
Acc. No: 012-4452-007  
THB:Krung Thai Bank PCL  
Siam Square Br.,416/1-2 Rama I Rd.,Pathumwan, BKK 10330  
Thailand

ORIGINAL

**Service Confirmation Number:** 6905338201

**Service Confirmation Date:** 12.12.2023

**Service Instrument:**

Model Number	Model Description	Serial Number	System Handle	Parent Asset
SYS-IM-7700-E	ICPMS 7700 System Enhanced		ICP MS 7700 (HPLC)	
G1316A	1260 Thermostatted Column Compartment	DEACN12300	ICP MS 7700 (HPLC)	SYS-IM-7700-E
G1329B	1260 Standard Autosampler	DEAAC11098	ICP MS 7700 (HPLC)	SYS-IM-7700-E
G1311B	1260 Quaternary Pump	DEAB704380	ICP MS 7700 (HPLC)	SYS-IM-7700-E
G3281A	Agilent 7700x ICP-MS	JP12091612	ICP MS 7700 (HPLC)	SYS-IM-7700-E

**Service Items:**



Item	Service/Part #	Description	Qty	Entitlement	Service Start	Service End
1000	EQQ	Enterprise Operational Qualification	1.00	Agreement Entitlement 100 % covered	12.12.2023	12.12.2023
1010	5185-5850	ICP-MS Checkout Solutions	1.00	Agreement Entitlement 100 % covered		

**Additional Information:**

**Service Confirmation Number:** 6905338201

**Service Confirmation Date:** 12.12.2023

**Service Information:**

<b>Problem Description:</b> WU-OQ-IM/HPLC-7700-5001143313		
<b>Service Provided:</b> Perform OQ Hardware control test CSD logon, Autosample , ISIS , Auto tune , BG and Stability. After done the instrument BKK_EL0026 calibrated pass all.		
<b>Service Overview Code:</b> Reason Code: Scheduled Service Diagnosis Code: Scheduled Service Resolution Code: Scheduled Service		
<b>Reported Hours:</b> 6.0	<b>Travel Hours:</b> 1.0	
<b>Customer Field Service Representative Name:</b> Panthep Kurasathain	<b>Customer Field Service Representative Signature:</b> 	<b>Date:</b> 12 Dec 2023
<b>Customer Name:</b> Supakwan Mak	<b>Customer Signature:</b> 	<b>Date:</b> 12 Dec 2023
<b>Additional Comments:</b>		



# Metrological Center

## SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110

Telephone : +66 2 586 5792-4 Fax : +66 2 586 5109

Website : www.scieco.co.th E-Mail : calibrate@scg.co.th

Certificate No. T231676

Page 1 of 6

## Certificate of Calibration

Equipment : HEATING BLOCK

Manufacturer : Environmental Express

Model : SC 196

Serial No. : 6974CECW3285

Customer Code : BKK\_EL0054

ID No. : T5306A3

Customer : ALS Laboratory Group (Thailand) Co.,Ltd.

104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan,

Khet Suan Luang, Bangkok 10250

Customer Location : Acid Digestion Lab

Date of Receipt : 13 September 2023

Calibrated By : Sanee Musikawan ( Site Calibration Manager )

Approved By :  / Sujjar Naknakred ( Site Calibration Manager )

Date of Issue : 26 SEP 2023

REVIEW BY	Tattaporn C.
APPROVED BY	Saenit N.
NEXT CAL. DATE	22/03/25

The uncertainties are for a confidence probability of approximately 95%.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standard laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Metrological Center.



# Metrological Center

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110

Telephone : +66 2 586 5792-4 Fax : +66 2 586 5109

Website : www.scieco.co.th E-Mail : calibrate@scg.co.th

Certificate No. T231676

Page 2 of 6

## Calibration Report

Equipment : HEATING BLOCK  
Date of Calibration : 22 September 2023  
Environment : Temperature : 21.8-23.1 °C  
Line Voltage : 221.6-226.3 V  
Relative Humidity : 55 - 65 %RH

### Condition of this results of calibration :

1. This equipment was calibrated by insert 20 standard thermocouples type T into its chamber , the other one standard thermocouples type T use for ambient temperature measurement . The calibration was done in according to WI-T20.

All data show below were final values and the initial data from customer request . The temperature scale used was based on ITS - 90 .

2. Reference Standard Instrument :

Instrument	Model	Instrument No.	Certificate No.	Due Date
TC	TYPE T	TN21-TN30	T230014	17 January 2024
TC	TYPE T	TN31-TN40	T230014	17 January 2024
DATA LOGGER	34970A	T151	T230014	17 January 2024

3. This certificate is traceable to :

National Institute of Metrology ( Thailand ) through Metrological Center ( NSC-TISI-TIS 17025 CALIBRATION 0244.)

4. Condition of calibrated item : good

Equipment Description :

Time Constant 2 Hour 20 Minute At 95 °C  
Fresh Air Damper ☐ Open ☐ Min ☐ Medium ☐ Max  
☐ Close  
☒ Not Available

5. Adjustment :

( ) without adjustment

( X ) after adjustment

Approved By. \_\_\_\_\_



# Metrological Center

## SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110

Telephone : +66 2 586 5792-4 Fax : +66 2 586 5109


Website : [www.scieco.co.th](http://www.scieco.co.th)

E-Mail : [calibrate@scg.co.th](mailto:calibrate@scg.co.th)

Certificate No. T231676

Page 3 of 6

## Calibration Report

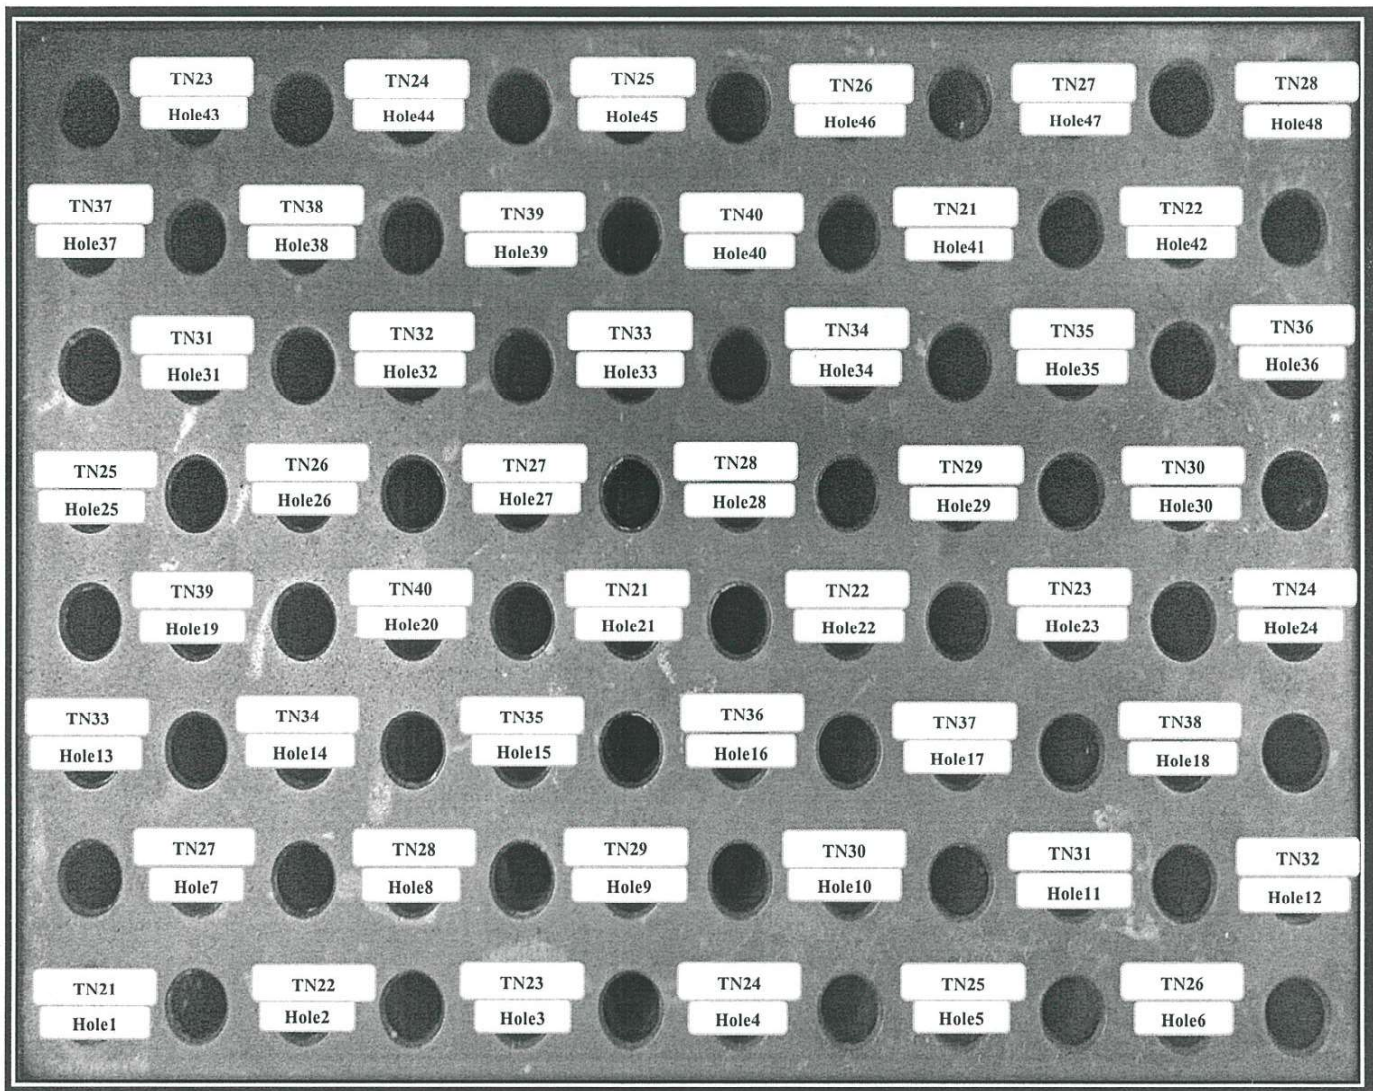

FRONT CONTROL

Approved By. \_\_\_\_\_



# Metrological Center

## SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110

Telephone : +66 2 586 5792-4 Fax : +66 2 586 5109

Website : www.scieco.co.th

E-Mail : calibrate@scg.co.th

Certificate No T231676

Page 4 of 6

## Calibration Report

### Measurement Results

Calibration Point		Average Standard Reading at each position ( ° C )					
R1 Hole1-Hole6		TN21	TN22	TN23	TN24	TN25	TN26
CAL POINT	Max	95.01	94.41	95.20	95.41	94.51	95.17
95	Min	94.57	93.95	94.75	94.92	94.00	94.72
	Average	94.79	94.18	94.98	95.17	94.26	94.95
R2 Hole7-Hole12		TN27	TN28	TN29	TN30	TN31	TN32
	Max	95.36	95.43	95.19	95.16	95.35	94.97
	Min	94.94	94.95	94.72	94.71	94.90	94.57
	Average	95.15	95.19	94.96	94.94	95.13	94.77
R3 Hole13-Hole18		TN33	TN34	TN35	TN36	TN37	TN38
	Max	95.37	95.50	95.22	95.21	95.33	95.31
	Min	94.99	95.09	94.78	94.82	94.88	94.96
	Average	95.18	95.30	95.00	95.02	95.11	95.13
R4 Hole19-Hole24		TN39	TN40	TN21	TN22	TN23	TN24
	Max	95.59	94.42	94.52	94.24	94.63	94.67
	Min	95.21	94.06	94.13	93.88	94.28	94.27
	Average	95.40	94.24	94.33	94.06	94.45	94.47
R5 Hole25-Hole30		TN25	TN26	TN27	TN28	TN29	TN30
	Max	95.19	95.38	92.93	95.30	95.14	95.03
	Min	94.83	95.03	92.56	94.95	94.79	94.70
	Average	95.01	95.20	92.75	95.12	94.96	94.87
R6 Hole31-Hole36		TN31	TN32	TN33	TN34	TN35	TN36
	Max	94.63	94.90	94.77	94.31	94.24	93.87
	Min	94.24	94.55	94.44	93.98	93.92	93.56
	Average	94.43	94.72	94.60	94.14	94.08	93.71
R7 Hole37-Hole42		TN37	TN38	TN39	TN40	TN21	TN22
	Max	94.30	94.44	94.04	93.81	94.89	95.35
	Min	93.95	94.05	93.67	93.48	94.39	94.90
	Average	94.13	94.24	93.86	93.65	94.64	95.12
R8 Hole43-Hole48		TN23	TN24	TN25	TN26	TN27	TN28
	Max	95.99	95.63	95.28	95.29	95.45	94.87
	Min	95.57	95.15	94.82	94.84	94.99	94.48
	Average	95.78	95.39	95.05	95.07	95.22	94.68

Approved By. \_\_\_\_\_

Certificate No T231676

Page 5 of 6

## Calibration Report

### Measurement Results

Calibration Point		Average Standard Reading at each position ( ° C )					
<b>R1 Hole1-Hole6</b>		<b>TN21</b>	<b>TN22</b>	<b>TN23</b>	<b>TN24</b>	<b>TN25</b>	<b>TN26</b>
CAL POINT	Max	105.23	104.32	105.43	105.25	104.44	105.27
105	Min	104.94	103.95	105.15	105.04	104.11	104.96
	Average	105.09	104.13	105.29	105.15	104.28	105.12
<b>R2 Hole7-Hole12</b>		<b>TN27</b>	<b>TN28</b>	<b>TN29</b>	<b>TN30</b>	<b>TN31</b>	<b>TN32</b>
	Max	105.30	105.12	105.18	105.22	105.12	105.16
	Min	105.11	104.92	104.96	105.00	104.92	104.97
	Average	105.20	105.02	105.07	105.11	105.02	105.06
<b>R3 Hole13-Hole18</b>		<b>TN33</b>	<b>TN34</b>	<b>TN35</b>	<b>TN36</b>	<b>TN37</b>	<b>TN38</b>
	Max	105.37	105.63	105.02	104.80	104.69	105.19
	Min	105.17	105.37	104.75	104.59	104.50	105.00
	Average	105.27	105.50	104.88	104.69	104.60	105.09
<b>R4 Hole19-Hole24</b>		<b>TN39</b>	<b>TN40</b>	<b>TN21</b>	<b>TN22</b>	<b>TN23</b>	<b>TN24</b>
	Max	105.31	104.43	106.41	104.71	105.63	105.82
	Min	105.08	104.22	106.15	104.41	105.37	105.56
	Average	105.19	104.33	106.28	104.56	105.50	105.69
<b>R5 Hole25-Hole30</b>		<b>TN25</b>	<b>TN26</b>	<b>TN27</b>	<b>TN28</b>	<b>TN29</b>	<b>TN30</b>
	Max	104.95	106.26	103.34	105.78	105.59	105.87
	Min	104.67	105.96	103.08	105.56	105.36	105.68
	Average	104.81	106.11	103.21	105.67	105.48	105.77
<b>R6 Hole31-Hole36</b>		<b>TN31</b>	<b>TN32</b>	<b>TN33</b>	<b>TN34</b>	<b>TN35</b>	<b>TN36</b>
	Max	104.75	104.86	104.80	105.20	104.50	104.39
	Min	104.54	104.63	104.59	105.00	104.32	104.18
	Average	104.65	104.75	104.69	105.10	104.41	104.28
<b>R7 Hole37-Hole42</b>		<b>TN37</b>	<b>TN38</b>	<b>TN39</b>	<b>TN40</b>	<b>TN21</b>	<b>TN22</b>
	Max	104.30	104.90	104.85	104.65	104.88	104.85
	Min	104.09	104.72	104.66	104.49	104.63	104.52
	Average	104.19	104.81	104.75	104.57	104.76	104.68
<b>R8 Hole43-Hole48</b>		<b>TN23</b>	<b>TN24</b>	<b>TN25</b>	<b>TN26</b>	<b>TN27</b>	<b>TN28</b>
	Max	105.71	105.85	105.39	105.61	105.42	105.19
	Min	105.45	105.61	105.14	105.27	105.18	104.94
	Average	105.58	105.73	105.27	105.44	105.30	105.07

Approved By. \_\_\_\_\_





# Metrological Center

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110

Telephone : +66 2 586 5792-4 Fax : +66 2 586 5109

Website : www.scieco.co.th

E-Mail : calibrate@scg.co.th

Certificate No. T231676

Page 6 of 6

## Calibration Report

### Measurement Results:

HEATING BLOCK			Temperature Distribution	
Setting (°C)	Reading (°C)		Stability ( $\pm$ °C)	Uncertainty ( $\pm$ °C)
	Min , Max	Average		
100.0	100.3 , 100.5	100.4	0.26	0.81
107.0	107.0 , 107.1	107.1	0.19	0.78

\* The quoted uncertainty exclude " uniformity "

The calibration result apply only the above calibrated item.

The result of test was found accurate as shown on date and place of test only.

The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor  $k$  which for a t-distribution, providing a level of confidence of approximately 95 % .

Approved By. \_\_\_\_\_



# Metrology

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110, Thailand.

Saraburi Tel : +66 3627 3096 Fax : +66 3627 3100

Bangkok Tel : +668 9205 6851 , +669 8247 2360  
Website : www.scieco.co.th E-Mail : calibrate@scg.com



Certificate No. T232160

Page 1 of 4

## Certificate of Calibration

Equipment : Chamber ( Cooling Room )

Manufacturer : KOLDTECH

Model : KM 320

Serial No. : TBN-1012061/05

Customer Code : BKK\_EN0167

ID No. : T2463A3

Customer : ALS Laboratory Group (Thailand) Co.,Ltd.


104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan,

Khet Suan Luang, Bangkok 10250



Customer Location : Laboratory

Date of Receipt : 29 November 2023

Calibrated By : Atiphong Rongrat ( Technician )

Approved By :  / Boonchai Suriyawong (Site Calibration Manager)

Date of Issue : 09 JAN 2024

REVIEW BY	<u></u>
APPROVED BY	<u></u>
NEXT CAL. DATE	<u>06/06/25</u>

The uncertainties are for a confidence probability of approximately 95%.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standard laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Metrology.

Certificate No. T232160

Page 2 of 4

## Calibration Report

**Equipment** : Chamber ( Cooling Room )  
**Date of Calibration** : 6 December 2023  
**Environment** : Temperature : 23.4-24.9 °C  
Line Voltage : 221.4-230.2 V  
Relative Humidity : 55 - 65 %RH

### Condition of this results of calibration :

- This equipment was calibrated by insert 16 standard thermocouples type T into its chamber , the other one standard thermocouples type T use for ambient temperature measurement . The calibration was done in according to WI-T20 ( based on ASTM E145-94 ( Reapproved 2001) and AS2853-1986 ).  
All data show below were final values and the initial data from customer request . The temperature scale used was based on ITS - 90 .

### 2. Reference Standard Instrument :

Instrument	Model	Instrument No.	Certificate No.	Due Date
TC	TYPE T	TN161-TN170	T230773	10 April 2024
TC	TYPE T	TN171-TN180	T230773	10 April 2024
DATA LOGGER	34970A	T149	T230773	10 April 2024

### 3. This certificate is traceable to :

National Institute of Metrology ( Thailand ) through Metrological Center ( NSC-TISI-TIS 17025 CALIBRATION 0244.)

### 4. Condition of calibrated item : good

Equipment Description :


Time Constant 1 Hour 30 Minute At 3 °C  
Fresh Air Damper ☐ Open ☐ Min ☐ Medium ☐ Max  
☐ Close  
☒ Not Available

### 5. Adjustment :

( X ) without adjustment


( ) after adjustment

Approved By. \_\_\_\_\_



**Certificate No. T232160**
**Page 3 of 4**

## Calibration Report

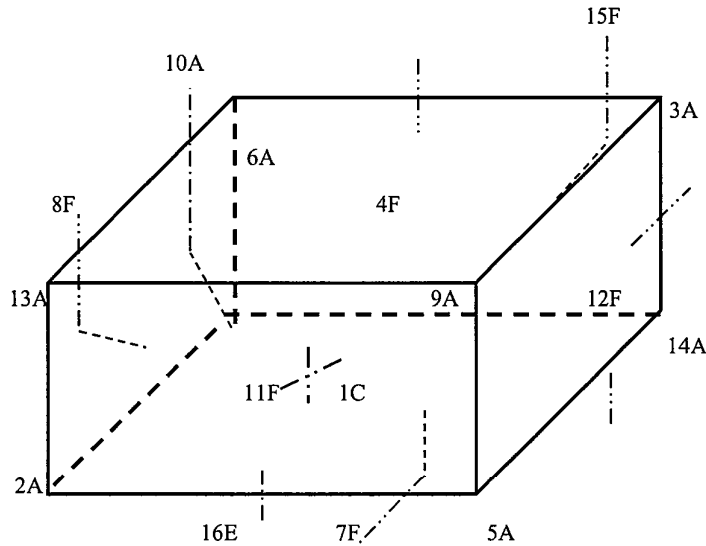

C = Centre , F = Centre of Face , A = Corner , E = Centre of Edge

1C = TN161	12F = TN172
2A = TN162	13A = TN173
3A = TN163	14A = TN174
4F = TN164	15F = TN175
5A = TN165	16E = TN176
6A = TN166	
7F = TN167	
8F = TN168	
9A = TN169	
10A = TN170	
11F = TN171	

Approved By. 

Certificate No. T232160

Page 4 of 4

## Calibration Report

### Measurement Results

Calibration Point	Average Standard Reading at each position (°C)											
	TN161	TN162	TN163	TN164	TN165	TN166	TN167	TN168	TN169	TN170	TN171	TN172
3.0	2.83	3.34	2.95	3.46	3.45	3.76	3.25	3.46	3.39	3.50	3.58	3.42
	TN173	TN174	TN175	TN176								
	3.33	3.39	3.15	3.43								

Chamber ( Cooling Room )			Temperature Distribution				
Setting (°C)	Reading (°C)		Average (°C)	Stability (± °C)	Uniformity (°C)	Uncertainty (± °C)	Coverage Factor <i>k</i>
	Min , Max	Average					
3.0	2.8 , 4.1	3.5	3.36	1.10	2.00	1.90	2.09

The calibration result apply only the above calibrated item.

The result of test was found accurate as shown on date and place of test only.

The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor *k* which for a t-distribution, providing a level of confidence of approximately 95 % .

Approved By. 



REVIEW BY	Chanath 2.
APPROVED BY	Sauntan M.
NEXT CAL. DATE	6/12/24

## Performance Verification Certificate for Mercury Analyzer

**PRODUCT ID** *Quicktrace M-8000 , Teledyne Leeman Labs*

**Equipment ID** *BKK\_EL0128 Mercury Analyzer  
S/N: US22133002*

*BKK\_EL0129 Autosampler  
S/N : 052222A560*

**Customer Name** *ALS Laboratory Group (Thailand) Co., Ltd.*

**Address** *104 Soi Pattana 40, Pattana Rd. Suan Luang, Suan Luang  
Bangkok 10250 Thailand*

**Date of Qualified** *December 6, 2023*

**Next Due date** *December 6, 2024*

This certifies for products which was performed in acceptable criteria specifications

<b>Autosampler &amp; Sample Introduction</b>	<b>PASSED</b>
<b>Analyzer</b>	<b>PASSED</b>
<b>Gas Liquid Separator &amp; Dryer</b>	<b>PASSED</b>
<b>CVAFS Detector</b>	<b>PASSED</b>
<b>Electronics/Mechanical</b>	<b>PASSED</b>
<b>Data station/PC</b>	<b>PASSED</b>
<b>Analytical test</b>	<b>PASSED</b>

**Provided by**

**Scientist Instrument Co.,Ltd.**  
113 Soi Ekachai 44, Ekachai Road  
Khlong Bang Phran, Bangbon  
Bangkok 10150 Thailand

**Certified by** *Thunraphol Sakdayos*

*Service Engineer*



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)  
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES  
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250  
TEL. 0-2717-3000-29 FAX. 0-2719-9484



Cert. No.: 23TM1103

Page : 1 of 3

## Certificate of Calibration

Equipment : Autoclave

Manufacturer : Sanyo

Model : MLS-3781

Serial No. : 830167

ID No. : BKK\_ML0037

Submitted by : ALS Laboratory Group (Thailand) Co.,Ltd.  
104 Phatthanakan 40, Phatthanakan Rd.,  
Khwaeng Phatthanakan, Khet Suan Luang,  
Bangkok 10250 Thailand

Location : Media Preparation Room

Received Order : 17 July 2023

Calibration Date : 17 July 2023

Ambient Temperature : ( 26 ± 10 ) °C

Relative Humidity : ( 50 ± 30 ) %

Calibrated by : Preecha Hlahib

Approved by :

Approved Signatory

( ) Pornthippa Tameyakul

( ) Malee Butkruea

(✓) Suwit Imjai

Issue Date : 24 July 2023

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written  
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.



Equipment : Autoclave  
Condition As-Received : Used Item  
Reference : 2307-0285OC-3

Cert. No.: 23TM1103

Page : 2 of 3

**Procedure Used :-**

Calibration were conducted using in-house calibration procedure CP-OT03 according to direct measurement method with Data Acquisition which connected with Thermocouple Type T

The temperature scale used was based on ITS-90.

**Condition of this result of calibration**

1. Reference standard instrument:-

<u>Instrument</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Traceable</u>	<u>Due Date</u>
1 ) Data Acquisition	MY57013823	23LM66	TPA	25 Mar 2024

2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certification is traceable to the International System of Unit.

4. This result of calibration covers laboratory autoclaves for the sterilization of goods and material which could be infected with organisms categorized as Hazard Group 1, 2 and 3\*\*

(\*\* = Categorization of pathogens according to hazard and categories of containment, second edition, 1990 )


It does not cover autoclaves for use with material infect with organisms in Hazard Group 4, for which complete containment and sterilization of infected condensate is considered to be essential.

This result of calibration does not apply to sterilizers or disinfectors used for medical, dental, pharmaceutical or veterinary purposes which are directly concerned with patient care, or those used for fabrics subjected to sterilization which are required to be dry at the end of cycle.

**Remark :** TPA : Technology Promotion Association ( Thailand - Japan )

**Result of Calibration :-** ( \* ) Without Adjustment

**Function of UUC\* :** Temperature Source

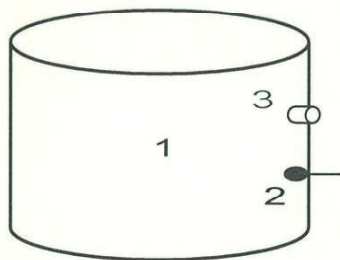

	<u>Environmental</u>		
	( °C )	( %R.H. )	( Volt )
<b>Beginning of Calibration</b>	22	53	220
<b>Finished of Calibration</b>	22	54	220

<u>Position</u>	<u>Description</u>	<u>Ref. Std. ID No.:</u>
1 =	Center of chamber	22-17TC-01
2 =	Temperature sensor	23-17TC-02
3 =	Exhaust port	19-17TC-03

*Yam*



Equipment : Autoclave

Cert. No.: 23TM1103

Condition As-Received : Used Item

Page : 3 of 3

Reference : 2307-0285OC-3

Result of Calibration :- ( \* ) Without Adjustment

Function of UUC\* : Temperature Source

Operating parameter Set : Temperature = 121 °C

Sterilization period = 15 minute

UUC* Setting ( °C )	UUC* Reading ( °C )	Position	Average* Standard Reading ( °C )	Stability ( ± °C )	Pressure Reading ( MPa )	Uncertainty ( ± °C )	Coverage Factor <i>k</i>
121	121	1	120.877	0.39	0.12	1.0	2
		2	120.870				
		3	120.866				

**Average\*** : The average of 30 values in each position.

**Stability** : One-half of the greatest maximum difference of measured temperature at any one probe.

**UUC\*** : Unit Under Calibration

Note : The reported uncertainty of measurement was included stability and excluded uniformity .

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

*Signature*



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)  
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES  
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250  
TEL. 0-2717-3000-29 FAX. 0-2719-9484



Cert. No.: 23TM1146

Page : 1 of 3

## Certificate of Calibration

Equipment : Incubator

Manufacturer : SHEL-LAB

Model : 1915A

Serial No. : 0200599

ID No. : BKK\_ML0010

Submitted by : ALS Laboratory Group (Thailand) Co.,Ltd.  
104 Phatthanakan 40, Phatthakan Rd.,  
Khawng Phatthanakan, Khet Suan Luang,  
Bangkok 10250 Thailand

Location : Incubation & Micrological Reading

Received Order : 17 July 2023

Calibration Date : 17 July 2023

Ambient Temperature : (  $26 \pm 10$  ) °C

Relative Humidity : (  $50 \pm 30$  ) %

Calibrated by : Man Pattanapongpaiboon

Approved by :

*Manu.*

Approved Signatory

( ) Pornthippa Tameyakul

( ☒ ) Malee Butkruea

( ) Suwit Imjai

Issue Date : 24 July 2023

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written  
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

A 0056489



Equipment : Incubator  
Condition As-Received : Used Item  
Reference : 2307-0285OC-1  
Procedure Used :-

Cert. No.: 23TM1146

Page : 2 of 3

Calibration were conducted using calibration procedure CP-OT02 according to direct measurement method with Data Acquisition which connected with Resistance Temperature Detector ( RTD ).

The temperature scale used was based on ITS-90.

**Condition of this result of calibration**

1. Reference standard instrument:-

<u>Instrument</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Traceable</u>	<u>Due Date</u>
1 ) Data Acquisition	MY49001451	23LM27	TPA	25 Feb 2024

2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certification is traceable to the International System of Unit.


**Remark :** TPA : Technology Promotion Association ( Thailand - Japan )

**Result of Calibration :-** ( \* ) Without Adjustment

**Function of UUC\* :** Temperature Source

**Fresh air setting :** Close

Environment during calibration		
	Beginning	Finished
Temp. ( °C )	24	24
REL.Humid. ( % )	54	56
AC Supply ( Volt )	221	223

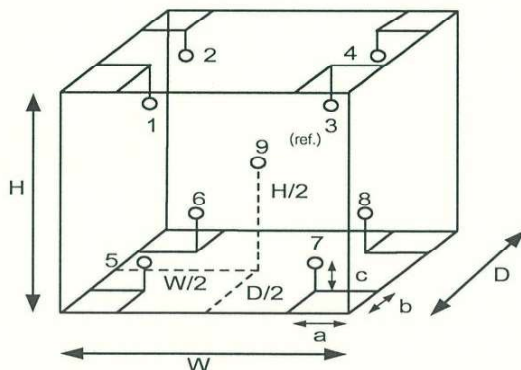

Position :	Ref. Std. ID No.:
1	19RTD-2/1
2	19RTD-2/2
3	19RTD-2/3
4	19RTD-2/4
5	19RTD-2/5
6	19RTD-2/6
7	19RTD-2/7
8	19RTD-2/8
9 (ref.)	19RTD-2/9

**Probe Installation Details :**

a = 10 cm  
b = 10 cm  
c = 10 cm

**Dimension of Chamber :**

D = 0.50 m  
W = 0.75 m  
H = 1.2 m  
Capacity = 0.45 m<sup>3</sup>

Malu .



Equipment : Incubator  
Condition As-Received : Used Item  
Reference : 2307-0285OC-1  
Result of Calibration :- ( \* ) Without Adjustment  
Function of UUC\* : Temperature Source  
Fresh air setting : Close

Cert. No.: 23TM1146

Page : 3 of 3

Calibration Point ( °C )	UUC* Setting ( °C )	UUC* Reading ( °C )	Temperature stability ( ± °C )	Temperature uniformity ( °C )	Overall Variation ( °C )	Coverage Factor <i>k</i>
35.0	35.0	35.0	0.055	0.30	0.44	2

Calibration Point ( °C )	Measured Temperature ( °C )									Uncertainty  ( ± °C )
	Position									
	1	2	3	4	5	6	7	8	9 (ref.)	
35.0	34.888	34.933	34.815	34.813	35.064	35.019	35.156	35.141	35.087	0.30

**Average\*** : The average of 30 values in each position.

**Temperature stability** : One-half of the greatest maximum difference of measured temperature at any one sensor.

**Temperature uniformity** : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.

**Overall Variation** : The Difference of the maximum and minimum measured temperatures throughout observation.

**UUC\*** : Unit Under Calibration

**Note** : The reported uncertainty of measurement was included stability and excluded uniformity .

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

Malu.



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)  
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES  
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250  
TEL.0-2717-3000-29 FAX.0-2719-9484



## Certificate of Calibration

Cert. No.: 24TM667

Page : 1 of 3

Equipment : Hot Air Oven  
Manufacturer : Binder  
Model : ED 240/E2  
Serial No. : 00-15533  
ID No. : BKK\_ML0013

Submitted by : ALS Laboratory Group (Thailand) Co.,Ltd.  
104 Phatthanakan 40, Phatthanakan Rd.,  
Khwaeng Phatthanakan, Khet Suan Luang,  
Bangkok 10250 Thailand

Location : Media Preparation Room

Received Order : 23 April 2024  
Calibration Date : 23 April 2024  
Ambient Temperature : ( 26 ± 10 ) °C  
Relative Humidity : ( 50 ± 30 ) %

Calibrated by : Tawatchai Pama

Approved by :

Approved Signatory

( ) Ponpan Paipim  
(✓) Suwit Imjai  
( ) Kunchit Promprat

Issue Date : 26 April 2024

REVIEW BY Sithichok T.  
APPROVED BY [Signature]  
NEXT CAL DATE 23/10/25

**The Uncertainties are for a confidence probability of approximately 95%**

This certificate may not be reproduced other than in full, except with the prior written  
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.



**Equipment :** Hot Air Oven  
**Condition As-Received :** Used Item  
**Reference :** 2404-0439OC-8  
**Procedure Used :-**

**Cert. No.:** 24TM667  
**Page :** 2 of 3

Calibration were conducted using calibration procedure CP-OT02 based on TLAS G-20 according to direct measurement method with Data Acquisition which connected with Thermocouple Type T.

The temperature scale used was based on ITS-90.

**Condition of this result of calibration**

1. Reference standard instrument:-

<u>Instrument</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Traceable</u>	<u>Due Date</u>
1 ) Data Acquisition	MY49001451	24LM44	TPA	17 Mar 2025

2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certification is traceable to the International System of Unit.


**Remark :** TPA : Technology Promotion Association ( Thailand - Japan )

**Result of Calibration :-** ( \* ) Without Adjustment

**Function of UUC\* :** Temperature Source

**Fresh air setting :** Close

Environment during calibration		
	Beginning	Finished
Temp. ( °C )	24	23
REL.Humid. ( % )	65	65
AC Supply ( Volt )	223	222

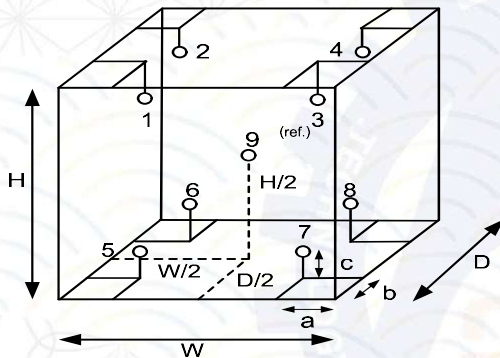

Position :	Ref. Std. ID No.:
1	24-19TC-01
2	24-19TC-02
3	24-19TC-03
4	24-19TC-04
5	24-19TC-05
6	24-19TC-06
7	24-19TC-07
8	24-19TC-08
9 (ref.)	24-19TC-09

**Probe Installation Details :**

a = 10 cm  
b = 10 cm  
c = 10 cm

**Dimension of Chamber :**

D = 0.50 m  
W = 0.80 m  
H = 0.60 m  
Capacity = 0.24 m<sup>3</sup>



**Equipment :** Hot Air Oven  
**Condition As-Received :** Used Item  
**Reference :** 2404-0439OC-8  
**Result of Calibration :-** ( \* ) Without Adjustment  
**Function of UUC\* :** Temperature Source  
**Fresh air setting :** Close

**Cert. No.:** 24TM667

**Page :** 3 of 3

Calibration Point ( °C )	UUC* Setting ( °C )	UUC* Reading ( °C )	Temperature stability ( ± °C )	Temperature uniformity ( °C )	Overall Variation ( °C )	Coverage Factor <i>k</i>
180	180	180	0.64	2.7	3.7	2

Calibration Point ( °C )	Measured Temperature ( °C )									Uncertainty  ( ± °C )
	Position									
	1	2	3	4	5	6	7	8	9 (ref.)	
180	181.009	181.511	180.922	181.359	181.217	183.659	181.664	181.986	181.474	1.5

**Average\* :** The average of 30 values in each position.

**Temperature stability :** One-half of the greatest maximum difference of measured temperature at any one sensor.

**Temperature uniformity :** The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.

**Overall Variation :** The Difference of the maximum and minimum measured temperatures throughout observation.

**UUC\* :** Unit Under Calibration

**Note :** The reported uncertainty of measurement was included stability and excluded uniformity .

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)  
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES  
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250  
TEL.0-2717-3000-29 FAX.0-2719-9484



## Certificate of Calibration

Cert. No.: 24TM469

Page : 1 of 3

Equipment : Water Bath  
Manufacturer : Memmert  
Model : WNE 45  
Serial No. : L712.0429  
ID No. : BKK\_ML0056

Submitted by : ALS Laboratory Group (Thailand) Co.,Ltd.  
104 Phatthanakan 40, Phatthanakan Rd.,  
Khwaeng Phatthanakan, Khet Suan Luang,  
Bangkok 10250 Thailand

Location : Incubation \$ Microbiological Reading

Received Order : 01 March 2024

Calibration Date : 01 March 2024

Ambient Temperature : ( 26  $\pm$  10 ) °C

Relative Humidity : ( 50  $\pm$  30 ) %

Calibrated by : Krisda Malee

Approved by :

Approved Signatory

( ) Pornthippa Tameyakul

( ) Unnopphol Harachai

(☒) Suwit Imjai

Issue Date : 4 March 2024

REVIEW BY *Sithichok T.*  
APPROVED BY *[Signature]*  
NEXT CAL DATE **01/03/25**

**The Uncertainties are for a confidence probability of approximately 95%**

This certificate may not be reproduced other than in full, except with the prior written  
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.



**Equipment :** Water Bath  
**Condition As-Received :** Used Item  
**Reference :** 2403-0001OC-1  
**Procedure Used :-**

**Cert. No.:** 24TM469  
**Page :** 2 of 3

Calibration were conducted using in-house calibration procedure CP-OT04 Based on ASTM E715 according to direct measurement method with Data Acquisition which connected with Industrial Platinum Resistance Thermometer ( IPRT ).

The temperature scale used was based on ITS-90.

**Condition of this result of calibration**

1. Reference standard instrument:-

<u>Instrument</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Traceable</u>	<u>Due Date</u>
1 ) Data Acquisition	MY57013711	23LM115	TPA	11 Jul 2024

2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certification is traceable to the International System of Unit.


**Remark :** TPA : Technology Promotion Association ( Thailand - Japan )

**Result of Calibration :-** ( \* ) Without Adjustment

**Function of UUC\* :** Temperature Source

**Heat transfer medium used :** Water

	<u>Environmental</u>		<u>AC Voltage Supply</u>
	( °C )	( %R.H. )	( Volt )
<b>Beginning of Calibration</b>	24	55	221
<b>Finished of Calibration</b>	23	56	220

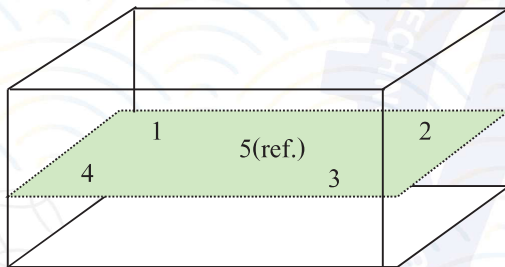

Front

<u>Position :</u>	<u>Ref. Std. ID No.:</u>
1	4803988-001
2	4803988-002
3	4803988-003
4	4803988-004
5(ref.)	4803988-005



**Equipment :** Water Bath  
**Condition As-Received :** Used Item  
**Reference :** 2403-0001OC-1  
**Result of Calibration :-** ( \* ) Without Adjustment  
**Function of UUC\* :** Temperature Source

**Cert. No.:** 24TM469

**Page :** 3 of 3

Calibration point ( °C )	UUC* Setting ( °C )	UUC* Reading ( °C )	Average* Standard Reading ( °C )					Uncertainty  ( ± °C )
			Position					
			1	2	3	4	5 (ref.)	
44.5	44.5	44.5	44.469	44.462	44.492	44.510	44.496	0.15
45.0	45.0	45.0	44.975	44.974	45.007	45.023	44.999	0.15

Calibration point ( °C )	Uniformity ( °C )	Stability ( ± °C )	Coverage Factor <i>k</i>
44.5	0.087	0.029	2
45.0	0.069	0.031	2

**Average\* :** The average of 30 values in each position.

**Uniformity :** The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.

**Stability :** One-half of the greatest maximum difference of measured temperature at any one probe.

**UUC\* :** Unit Under Calibration

**Note :** The reported uncertainty of measurement was included stability and excluded uniformity.

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-



**TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)**  
**CORPORATE SERVICES 3 : EQUIPMENT CALIBRATION AND TESTING SERVICES**


534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250



TEL. 0-2717-3000 FAX. 0-2719-9484

**Cert.No.:** 23TW243

**Page.:** 1 of 2

## Certificate of Testing

<b>Equipment :</b>	DO Meter
<b>Manufacturer :</b>	YSI
<b>Model :</b>	5000-230V
<b>Serial No. :</b>	09J101147
<b>ID No. :</b>	BKK_EN0017
<b>Received Date :</b>	15 November 2023
<b>Test Date :</b>	16 November 2023
<b>Reference :</b>	2311-0505DSC-4
<b>Submitted by :</b>	ALS Laboratory Group (Thailand) Co.,Ltd. 104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan, Khet Suan Luang, Bangkok 10250 Thailand
<b>Laboratory Condition :</b>	Temperature ( $25 \pm 5$ ) °C Humidity ( $50 \pm 20$ ) %
<b>Test Procedure :</b>	In - house method : CP-CH9 by Comparison Technique with Azide Modification Method
<b>Tested by :</b>	Walalak Sirithean
<b>Approved by :</b>	 Approved Signatory
<input checked="" type="checkbox"/> Saithip Meangmai <input type="checkbox"/> Warakorn Lergagtrakul <input type="checkbox"/> Ponpan Paipim	
<b>Issue Date :</b>	17 November 2023

REVIEW BY	
APPROVED BY	
NEXT CAL. DATE	16/05/25



Cert.No.: 23TW243

Page.: 2 of 2

**Condition of this result of calibration**

1. Reference Standard Instruments :

This certification is traceable to the International System of Unit through the reference standards laboratory of Industrial Calibration Center, Technology Promotion Association (Thailand-Japan).

<u>Instruments</u>	<u>Serial No.</u>	<u>ID No.</u>	<u>Certificate No.</u>	<u>Due Date</u>
1) Burette	-	130BU10	23CG1172	22 Mar 2025
2) Balance	1124013382	140RC006	23MM18	20 Feb 2024

2. Standard Material :-

<u>Material</u>	<u>Manufacturer</u>	<u>Lot.No.</u>	<u>Assay</u>
Sodium Thiosulfate pentahydrate	Merck	AM1763316	100.2%

**Result :** Dissolved Oxygen Meter Adjustment With Air 100 %

Dissolved Oxygen Probe No.: 16K100498

<b>Titration Method (Azide Modification Method) (mg/L)</b>	<b>DO Meter Reading (mg/L)</b>	<b>Standard Deviation (mg/L)</b>
8.18	8.18	0.0055

This report was certified only for the instrument we tested. It is allowable to use for study the system efficiency, The environmental impact control and present to organization it may concerned. Intend to use for advertising and referral purpose is prohibited. This report may not be reproduced other in full, without written approval of the laboratory

-o0o-

*Santhip*

**a 1190297**



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)  
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES  
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250  
TEL. 0-2717-3000-29 FAX. 0-2719-9484



Cert. No.: 23LM192

Page.: 1 of 2

## Certificate of Calibration

**Equipment :** DO Meter with Sensor

**Manufacturer :** YSI

**Model :** 5000-230V

**Serial No. :** 09J101147

**ID No. :** BKK\_EN0017

**Submitted by :** ALS Laboratory Group (Thailand) Co.,Ltd.  
104 Phatthanakan 40, Phatthanakan Rd.,  
Khwaeng Phatthanakan, Khet Suan Luang,  
Bangkok 10250 Thailand

**Location :** TPA Chemistry Calibration Laboratory

**Received Order :** 15 November 2023


**Calibrated Date :** 16 November 2023

**Ambient Temperature :** ( 26 ± 10 ) °C

**Relative Humidity :** ( 50 ± 30 ) %

**AC Line Voltage :** ( 220 ± 22 ) V

**Calibrated by :** Kunchit Promprat

**Approved by :**   
Approved Signatory

( ) Pornthippa Tameyakul  
( ) Ponpan Paipim  
(✓) Suwit Imjai

**Issue Date :** 17 November 2023

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written  
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

A 0060730



**Equipment :** DO Meter with Sensor  
**Condition As-Received :** Used Item  
**Reference :** 2311-0505DSC-10

**Cert. No.:** 23LM192

**Page.:** 2 of 2

**Procedure Used :-**

Calibration were conducted using in-house calibration procedure CP-OT01 according to comparison with Industrial Platinum Resistance Thermometer ( IPRT ) into Temperature Bath.

The temperature scale used was based on ITS-90.

**Condition of this result of calibration**

1. Reference standard instrument:-

<u>Instrument</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Traceable</u>	<u>Due Date</u>
1) Digital Thermometer	3240076	23I305	TPA	15 Mar 2024

2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certification is traceable to the International System of Unit.

**Remark :** TPA : Technology Promotion Association ( Thailand - Japan )

**Result of Calibration :-** ( \* ) Without Adjustment

**Function :** Temperature measurement.

This instrument was connected with temperature sensor, S/N.: 16K100498

<u>Calibration Point</u> ( °C )	<u>Immersion Depth</u> ( mm )	<u>Standard Temperature</u> ( °C )	<u>UUC* Reading</u> ( °C )	<u>Error</u> ( °C )	<u>Uncertainty</u> ( ± °C )	<u>Coverage Factor</u> <i>k</i>
20.0	60	19.997	19.93	-0.067	0.15	2.00

**UUC\* :** Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

*Yunt*

**a 1190298**



# QUALITY CALIBRATION CO.,LTD.

235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160

Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

www.qcalibration.com



CERTIFICATE No : 24T2852  
REFERENCE No : 72619-8

PAGE : 1 OF 2

## Certificate of Calibration

EQUIPMENT : COOLED INCUBATOR  
MANUFACTURER : MEMMERT  
MODEL : ICP750  
SERIAL No : F819.0021  
ID No : BKK\_EN0304  
CONDITION AS RECEIVED : USED ITEM  
SUBMITTED BY : ALS LABORATORY GROUP (THAILAND) CO., LTD.  
104 PHATTHANAKAN 40, PHATTHANAKAN  
RD.,KHWAEANG PHATTHANAKAN,KHET SUAN  
LUANG, BANGKOK 10250, THAILAND

REVIEW BY

*Jinda K*

APPROVED BY

*Siriluk P.*

NEXT CAL. DATE

*20/03/25*

CALIBRATED BY : CHAICHARN CH.

CALIBRATION DATE : 20-Mar-24

APPROVED BY : *[Signature]*  
PONGSAK J.

ISSUED DATE : 21-Mar-24

RECEIVED DATE : 20-Mar-24



CERTIFICATE No : 24T2852

PAGE : 2 OF 2

## Calibration Report

EQUIPMENT : COOLED INCUBATOR  
MANUFACTURER : MEMMERT  
MODEL : ICP750  
ID No : BKK\_EN0304  
RECEIVED DATE : 20-Mar-24  
AMBIENT TEMPERATURE : 26 °C ± 1 °C

S/N : F819.0021  
CALIBRATION DATE : 20-Mar-24  
RELATIVE HUMIDITY : 54 %RH ± 10 %RH

### CONDITION OF THIS RESULTS OF CALIBRATION


1. THIS INSTRUMENT WAS CALIBRATED ACCORDING TO TLAS G-20 BY COMPARISON WITH CALIBRATED THERMOCOUPLE TYPE K UNDER NO LOAD CONDITION. THE THERMOCOUPLES WERE PLACED ON NINE POINTS AND LOCATED ONE THERMOCOUPLE IN EACH OF THE EIGHT CORNERS OF THE CHAMBER AND WAS AWAY FROM THE EACH WALL OF 5 cm TO 10 cm. AND PLACED THE NINTH THERMOCOUPLE WITHIN 2.5 cm. OF THE GEOMETRIC CENTER OF THE CHAMBER. THE UNIFORMITY WAS MEASURED BETWEEN REFERENCE PROBE AND OTHER PROBES AT THE SAME TIME.

2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) DATA LOGGER WITH TC TYPE K	HYDRA 2635A	7286308	23T6641	14-Jul-24

3. THE CERTIFICATE IS VALID FOR THE ITEM CALIBRATED AS SHOWN ON THE DATE AND PLACE OF CALIBRATION ONLY.  
4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.  
5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-  
- NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH QUALITY CALIBRATION CO.,LTD.

### RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

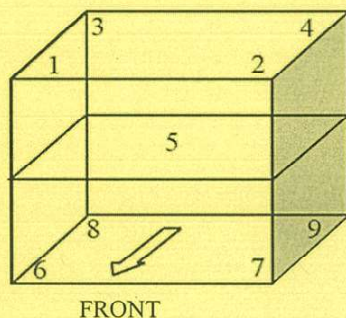

#### GENERAL INFORMATION

Overall Ambient Temperature around the Chamber (°C) variation : 1
Overall Line Voltage (V) variation : 5
Instrument Condition : Normal

#### CHAMBER PERFORMANCE

Controller Temperature (°C)	Indicating Temperature (°C)	Temperature Stability (±°C)	Temperature Uniformity (°C)	Overall Variation (°C)
20.0	20.0	0.16	0.21	0.41

#### TEMPERATURE MEASUREMENT ACCURACY TEST

Controller Temp (°C)	Indicating Temp (°C)	Measured Temperature (°C) at Spread Locations									Uncertainty (±°C)
		#1	#2	#3	#4	Ref. 5	#6	#7	#8	#9	
20.0	20.0	19.88	19.93	19.87	19.86	19.98	19.94	19.94	19.89	19.91	0.42

NOTE 1 : THE UNCERTAINTY OF MEASUREMENT EXCLUDED TEMPERATURE UNIFORMITY OF THE CHAMBER.

NOTE 2 : LOCATION 5 WAS REFERENCE LOCATION.

NOTE 3 : THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA.

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR  $k=2$ , PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.  
END OF CALIBRATION REPORT



## Certificate of Calibration

Cert.No.: 24CG952

Page.: 1 of 2

**Equipment :** Burette  
**Capacity :** 50 mL  
**Serial No. :** -  
**ID. No. :** BKK\_EN0171  
**Manufacturer :** Witeg  
**Made in :** Germany  
**Submitted by :** ALS Laboratory Group (Thailand) Co.,Ltd.  
104 Phatthanakan 40, Phatthanakan Rd.,  
Khwaeng Phatthanakan, Khet Suan Luang,  
Bangkok 10250 Thailand  
**Ambient Temperature :** (20 ± 2.5) °C  
**Relative Humidity :** (50 ± 10) %  
**Barometric Pressure :** 760 mmHg  
**Calibration Procedure :** ASTM E 542 - 01  
**Calibrated by :** Natcha Chayingcheiw

**Approved by :**

Approved Signatory

- ( ) Unnopphol Harachai  
(✓) Srisuda Khamtha  
( ) Sa-ngeunkam Wongsai

**Issue Date :**

27 February 2024

REVIEW BY ..... *Siriluk P.* .....  
APPROVED BY ..... *Kark Anh.* .....  
NEXT CAL DATE..... **27/08/25** .....

**The Uncertainties are for a confidence probability of approximately 95%**

This certificate may not be reproduced other than in full, except with the prior written  
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.



**Equipment :** Burette  
**Received Date :** 23 February 2024  
**Condition As-Received :** New Item  
**Calibration Date :** 27 February 2024  
**Reference :** 2402-0757DSC-1

**Cert.No.:** 24CG952

**Page.:** 2 of 2

**Condition of this result of calibration**

1. Reference Standard Instruments :

<u>Instruments</u>	<u>Model</u>	<u>Serial No.</u>	<u>ID. No.</u>	<u>Certificate No.</u>	<u>Traceability</u>	<u>Due date</u>
1) Balance	XP205DR	1126143764	140RC004	23MM538	TPA	15 Sep 2024
2) Thermo-Hygrograph	THDX-CE	00016540	140EC001	23H1275	TPA	09 June 2024
3) Thermometer	-	0834181	140EC005	23I948	TPA	10 Aug 2024

This certification is traceable to SI Unit

2. The certificate is valid only to the item calibrated on date and place of calibration.  
3. True value is converted to true volume at the standard temperature of 20 °C

**Calibration result :**

<b>Nominal capacity ( mL )</b>	<b>Reading ( mL )</b>	<b>Uncertainty ( ± mL )</b>	<b>k Factor</b>
50	50.0032	0.010	2.00

**Remark** mL = cm<sup>3</sup>

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor  $k$  , providing a level of confidence of approximately 95 %.

-o0o-



# Metrological Center

## SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110

Telephone : +66 2 586 5792-4 Fax : +66 2 586 5109

Website : www.scieco.co.th E-Mail : calibrate@scg.co.th

Certificate No. T240741

Page 1 of 5

## Certificate of Calibration

Equipment : HOT BLOCK

Manufacturer : Environmental Express

Model : B3000- 240

Serial No. : 2017CODW116

Customer Code : BKK\_EN0222

ID No. : T6769A4

Customer : ALS Laboratory Group (Thailand) Co.,Ltd.

104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan,

Khet Suan Luang, Bangkok 10250

Customer Location : Wet Chemistry Lab2

Date of Receipt : 11 April 2024

Calibrated By : Sanee Musikawan ( Site Calibration Manager )

Approved By :  / Sujjar Naknakred (Site Calibration Manager)

Date of Issue : 23 APR 2024

REVIEW BY	<u>Jinda K</u>
APPROVED BY	<u>Siriluk P.</u>
NEXT CAL. DATE	<u>22/04/25</u>

The uncertainties are for a confidence probability of approximately 95%.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standard laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Metrological Center.



# Metrological Center

## SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110

Telephone : +66 2 586 5792-4 Fax : +66 2 586 5109

Website : www.scieco.co.th E-Mail : calibrate@scg.co.th

Certificate No. T240741

Page 2 of 5

## Calibration Report

Equipment : HOT BLOCK  
Date of Calibration : 22 April 2024  
Environment : Temperature : 22.9-24.4 °C  
Line Voltage : 222.7-227.8 V  
Relative Humidity : 55 - 65 %RH

### Condition of this results of calibration :

1. This equipment was calibrated by insert 20 standard thermocouples type T into its chamber , the other one standard thermocouples type T use for ambient temperature measurement . The calibration was done in according to WI-T20 ( based on ASTM E145-94 ( Reapproved 2001) and AS2853-1986 ).

All data show below were final values and the initial data from customer request . The temperature scale used was based on ITS - 90 .

2. Reference Standard Instrument :

Instrument	Model	Instrument No.	Certificate No.	Due Date
TC	TYPE T	TN21-TN30	T240235	17 February 2025
TC	TYPE T	TN31-TN40	T240235	17 February 2025
DATA LOGGER	34970A	T195	T240235	17 February 2025

3. This certificate is traceable to :

National Institute of Metrology ( Thailand ) through Metrological Center ( NSC-TISI-TIS 17025 CALIBRATION 0244.)

4. Condition of calibrated item : good

Equipment Description :

Time Constant 1 Hour 10 Minute At 150 °C  
Fresh Air Damper ☐ Open ☐ Min ☐ Medium ☐ Max  
☐ Close  
☒ Not Available

5. Adjustment :

( X ) without adjustment


( ) after adjustment

Approved By. \_\_\_\_\_

Certificate No. T240741

Page 3 of 5

## Calibration Report

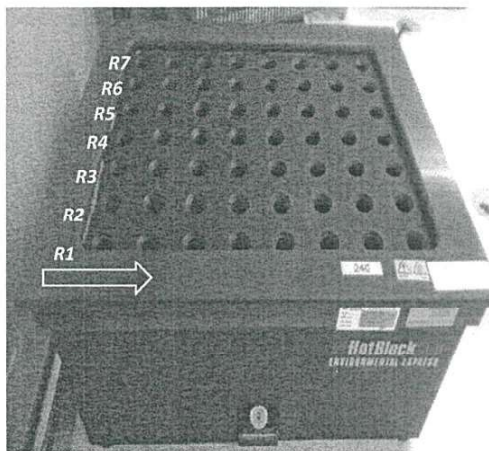

Row	Hole							
R7	H49	H50	H51	H52	H53	H54	H55	H56
R6	H41	H42	H43	H44	H45	H46	H47	H48
R5	H33	H34	H35	H36	H37	H38	H39	H40
R4	H25	H26	H27	H28	H29	H30	H31	H32
R3	H17	H18	H19	H20	H21	H22	H23	H24
R2	H9	H10	H11	H12	H13	H14	H15	H16
R1	H1	H2	H3	H4	H5	H6	H7	H8

H: STANDARD THERMOCOUPLE TYPE T

H1	=	TN21	H9	=	TN29	H17	=	TN37	H25	=	TN25	H33	=	TN33	H41	=	TN21	H49	=	TN29
H2	=	TN22	H10	=	TN30	H18	=	TN38	H26	=	TN26	H34	=	TN34	H42	=	TN22	H50	=	TN30
H3	=	TN23	H11	=	TN31	H19	=	TN39	H27	=	TN27	H35	=	TN35	H43	=	TN23	H51	=	TN31
H4	=	TN24	H12	=	TN32	H20	=	TN40	H28	=	TN28	H36	=	TN36	H44	=	TN24	H52	=	TN32
H5	=	TN25	H13	=	TN33	H21	=	TN21	H29	=	TN29	H37	=	TN37	H45	=	TN25	H53	=	TN33
H6	=	TN26	H14	=	TN34	H22	=	TN22	H30	=	TN30	H38	=	TN38	H46	=	TN26	H54	=	TN34
H7	=	TN27	H15	=	TN35	H23	=	TN23	H31	=	TN31	H39	=	TN39	H47	=	TN27	H55	=	TN35
H8	=	TN28	H16	=	TN36	H24	=	TN24	H32	=	TN32	H40	=	TN40	H48	=	TN28	H56	=	TN36

 Approved By. 



# Metrological Center

## SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110

Telephone : +66 2 586 5792-4 Fax : +66 2 586 5109

Website : [www.scieco.co.th](http://www.scieco.co.th)

E-Mail : [calibrate@scg.co.th](mailto:calibrate@scg.co.th)

Certificate No. T240741

Page 4 of 5

## Calibration Report

### Measurement Results

			Average Standard Reading at each position ( ° C )									
Calibration Point			TN21	TN22	TN23	TN24	TN25	TN26	TN27	TN28	TN29	TN30
Point	Setting	Max	150.38	149.73	150.12	150.36	150.56	150.00	150.48	150.25	150.56	149.59
150	150.0	Min	150.13	149.47	149.87	150.16	150.31	149.77	150.25	150.02	149.41	149.41
		Average	150.23	149.59	149.96	150.24	150.41	149.87	150.36	150.12	150.45	149.51
			TN31	TN32	TN33	TN34	TN35	TN36	TN37	TN38	TN39	TN40
		Max	150.17	150.28	150.28	150.37	150.09	149.96	149.86	149.75	150.63	150.13
		Min	149.94	150.03	150.01	150.18	149.88	149.69	149.68	149.57	150.41	149.96
		Average	150.04	150.14	150.13	150.27	149.98	149.81	149.77	149.65	150.51	150.03
			TN21	TN22	TN23	TN24	TN25	TN36	TN27	TN28	TN29	TN30
		Max	150.28	150.18	149.87	149.57	150.18	149.90	150.59	149.66	150.39	150.08
		Min	150.00	149.94	149.67	149.39	149.88	149.58	150.32	149.34	150.11	149.84
		Average	150.14	150.07	149.77	149.49	150.04	149.75	150.48	149.52	150.26	149.97
			TN31	TN32	TN33	TN34	TN35	TN36	TN37	TN38	TN39	TN40
		Max	150.38	149.71	150.18	149.97	150.03	150.05	150.21	150.07	150.02	149.92
		Min	150.12	149.49	149.87	149.66	149.71	149.71	149.89	149.79	149.76	149.73
		Average	150.26	149.61	150.04	149.82	149.90	149.89	150.05	149.94	149.91	149.84
			TN21	TN22	TN23	TN24	TN25	TN26	TN27	TN28	TN29	TN30
		Max	150.37	150.20	150.20	150.44	150.67	149.85	150.31	149.90	150.36	149.62
		Min	150.11	149.99	150.04	150.26	150.49	149.69	150.12	149.78	150.20	149.40
		Average	150.25	150.12	150.14	150.34	150.57	149.78	150.20	149.83	150.29	149.52
			TN31	TN32	TN33	TN34	TN35	TN36				
		Max	150.18	150.02	149.95	150.26	149.92	149.69				
		Min	150.06	149.88	149.79	150.12	149.80	149.58				
		Average	150.13	149.95	149.89	150.18	149.84	149.64				

Approved By. \_\_\_\_\_



# Metrological Center

## SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110

Telephone : +66 2 586 5792-4 Fax : +66 2 586 5109

Website : www.scieco.co.th

E-Mail : calibrate@scg.co.th

Certificate No. T240741

Page 5 of 5

## Calibration Report

### Measurement Results

HOT BLOCK			Temperature Distribution	
Setting (°C)	Reading (°C)		Stability ( $\pm$ °C)	Uncertainty ( $\pm$ °C)
	Min , Max	Average		
150.0	150 , 150.1	150.0	0.20	0.83

The calibration result apply only the above calibrated item.

The result of test was found accurate as shown on date and place of test only.

The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor  $k=2$  , providing a level of confidence of approximately 95 % .

Approved By. \_\_\_\_\_

# Certificate of Calibration

Number of Page(s) 1 of 3

**Certificate No.** BSCC-UV-374/24  
**Equipment** UV/Vis Spectrophotometer  
**Model** UV-1800  
**Manufacturer** Shimadzu  
**Serial No.** A11454908533 CD  
**ID No.** BKK\_EN0018  
**Date of receipt** 13 September 2024  
**Date of calibration** 13 September 2024  
**Date of issue** 13 SEP 2024

REVIEW BY

*Jinda K*

APPROVED BY

*Siriluk P*

NEXT CAL. DATE

*13/9/2025*

**Customer name** ALS Laboratory Group (Thailand) Co., Ltd.

**Address** 104 Soi Phattanakan 40, Phattanakan Road, Phattanakan, Suan Luang, Bangkok 10250

**Temperature** (25.3 - 26.7) °C (On site)  
**Humidity** (50.4 - 55.9) %RH (On site)

**Equipment condition** Good Operation

**Calibration Location** Organic Preparation Lab

**Calibration Procedure** In-house method WI-UV-702-01 based on ASTM E275-01

**Traceability** Wavelength Accuracy is traceable to certificate No. 106372 and 106371  
Photometric Accuracy is traceable to certificate No. 106364 and 111398  
Stray Light is traceable to certificate No. 106377  
The above certificate are traceable to SI unit through Sarnia Scientific Ltd.  
(UKAS accredited calibration laboratory NO. 0659)

**Calibrated by** Mr.Wanchana Janloey

Approved by



**Mr.Sonthi Temboonsakdi**  
Service Manager

The above results are valid exclusively for the calibrated item(s) as mention in this report / certificate.  
Advertising the report / Certificate and publicity of the results are prohibited and also shall not be reproduced  
except in full, without written approval of the Bara Scientific Co., Ltd.

# Certificate of Calibration

Certificate No. **BSCC-UV-374/24**

Number of Page(s) **2 of 3**

## Calibration Results:

### 1.Wavelength Accuracy

Certified Wavelength (nm)	UUC (nm)	Error (nm)	Uncertainty ( $\pm$ nm)
241.70	241.55	-0.15	0.18
334.02	333.85	-0.17	0.18
418.53	418.57	0.04	0.18
572.99	572.97	-0.02	0.18
879.41	879.17	-0.24	0.18

### 2.Photometric Accuracy (UV)

Wavelength (nm)	Certified Absorbance (A)	UUC (A)	Error (A)	Uncertainty ( $\pm$ A)
235	0.0000	0.0000	0.0000	0.0075
	0.7171	0.7169	-0.0002	0.0075
257	0.0000	0.0000	0.0000	0.0075
	0.8354	0.8345	-0.0009	0.0075
313	0.0000	0.0000	0.0000	0.0075
	0.2786	0.2781	-0.0005	0.0075
350	0.0000	0.0000	0.0000	0.0075
	0.6199	0.6194	-0.0005	0.0075

\*CNR = Customer not request

The above results are valid exclusively for the calibrated item(s) as mention in this report / certificate.  
Advertising the report / Certificate and publicity of the results are prohibited and also shall not be reproduced  
except in full, without written approval of the Bara Scientific Co., Ltd.

# Certificate of Calibration

Certificate No. **BSCC-UV-374/24**

Number of Page(s) **3 of 3**

## Calibration Results:

### 3. Photometric Accuracy (Visible)

Wavelength (nm)	Certified Absorbance (A)	UUC (A)	Error (A)	Uncertainty ( $\pm A$ )
420.0	0.0000	0.0000	0.0000	0.0042
	0.5761	0.5765	0.0004	0.0042
	0.7119	0.7105	-0.0014	0.0042
	1.0189	1.0174	-0.0015	0.0042
440.0	0.0000	0.0000	0.0000	0.0042
	0.5610	0.5613	0.0003	0.0042
	0.7001	0.6984	-0.0017	0.0042
	1.0026	1.0011	-0.0015	0.0042
465.0	0.0000	0.0000	0.0000	0.0042
	0.5235	0.5232	-0.0003	0.0042
	0.6614	0.6598	-0.0016	0.0042
	0.9456	0.9444	-0.0012	0.0042
546.1	0.0000	0.0000	0.0000	0.0042
	0.5249	0.5245	-0.0004	0.0042
	0.6975	0.6956	-0.0019	0.0042
	1.0009	0.9994	-0.0015	0.0042
590.0	0.0000	0.0000	0.0000	0.0042
	0.5590	0.5586	-0.0004	0.0042
	0.7725	0.7708	-0.0017	0.0042
	1.1125	1.1114	-0.0011	0.0042
635.0	0.0000	0.0000	0.0000	0.0042
	0.5666	0.5666	0.0000	0.0042
	0.7620	0.7604	-0.0016	0.0042
	1.0982	1.0971	-0.0011	0.0042

\*CNR = Customer not request

### 4. Stray Light\*

Standard cut-off wavelength (nm)	Unit Under Calibration(UUC)		
	Wavelength (nm)	Transmission (%T)	Absorbance (A)
200.85 $\pm$ 0.11nm	199.58	0.9520	2.0217

The Stray light transmission reference is less than 1.0%T and Stray light absorbance reference is greater than 2.00A

\*Stray Light not NSC-ONSC Accredited.

The measurement uncertainty is base on a standard uncertainty multiplied by a coverage factor k=2 providing a level of confidence of approximately 95%.

**\*\*\*End of Certificate\*\*\***

The above results are valid exclusively for the calibrated item(s) as mention in this report / certificate.  
Advertising the report / Certificate and publicity of the results are prohibited and also shall not be reproduced except in full, without written approval of the Bara Scientific Co., Ltd.



## Certificate of Calibration

**Equipment:** CONDUCTIVITY METER **Certificate No.:** C24230292  
**Model:** ORION STAR A215 **Issued Date:** 25 December 2023  
**Serial No. (or ID.):** X58031 **Job No.:** WO-00012682  
**Manufacturer:** Thermo Scientific **Page:** 1 of 2  
**Electrode Serial No.** YV1-18416 **Model :** ORION 013005MD **Brand :** Thermo Scientific  
**Condition:** In Condition

**Customer:** ALS Laboratory Group (Thailand) Co., Ltd.  
 104 Soi Pattanakarn 40, Pattanakarn Rd.,  
 Suan Luang, Bangkok 10250 Thailand

REVIEWED BY Simluk P.  
 APPROVED BY [Signature]  
 NEXT CAL. DATE 25/12/24

**Environment Condition:** Temperature 21.7 °C ± 0.1 °C  
 Humidity 53.7 %RH ± 0.1 %RH


**Calibration Place:** ALS Laboratory Group (Thailand) Co., Ltd.. ( Wet Chemistry Lab 2 )  
 104 Soi Pattanakarn 40, Pattanakarn Rd.,  
 Suan Luang, Bangkok 10250 Thailand

**Calibration By:** Mr.Siwapan Srijan  
**Calibration Date:** 25 December 2023  
**The Method used:** In house method, CAL-WI-49, base on ASTM D 1125-14 and D 5391-14  
**Traceability:** This certificate is traceable to the SI Units maintained by CRM of NIST(SRM) through CPA chem Co., Ltd. (ISO/IEC 17034) Certificate No. 890590, 890591, 890592



(Mr.Siwapan Srijan)

Person in charge



(Mr.Nitinun Srihawan)

Authorized signatory

This certificate is issued the units of measurement according to the International System of Units (SI). It provides traceability of measurement to international or national standard or other recognized national standard laboratories.

The measurement uncertainty stated is the expanded uncertainty which is obtained from the standard uncertainty multiplied by the coverage factor (k=2) to provide a level of confidence of approximately 95%. It is determined in accordance with the Guide to Expression of Uncertainty in Measurement (GUM).

These results may be affected by deviations from specified conditions. The results relate only to the items tested, calibrated or sampled. The report shall not be reproduced except in full without approval of DKSH Technology Limited.

**Calibration Results:**
**Before Adjustment**

Standard Conductivity Solution	Unit Under Calibration Reading	Correction	Coverage Factor ( k )	Uncertainty ( ± )
84.000 $\mu\text{S/cm}$	92.64 $\mu\text{S/cm}$	-8.640 $\mu\text{S/cm}$	2.00	0.68 $\mu\text{S/cm}$
1413.0 $\mu\text{S/cm}$	1423 $\mu\text{S/cm}$	-10.0 $\mu\text{S/cm}$	2.00	11 $\mu\text{S/cm}$
12.880 $\text{mS/cm}$	12.81 $\text{mS/cm}$	0.070 $\text{mS/cm}$	2.00	0.10 $\text{mS/cm}$

**After Adjustment ;    at    84.0  $\mu\text{S/cm}$ , 1413  $\mu\text{S/cm}$ , 12.88  $\text{mS/cm}$** 

Standard Conductivity Solution	Unit Under Calibration Reading	Correction	Coverage Factor ( k )	Uncertainty ( ± )
84.000 $\mu\text{S/cm}$	84.03 $\mu\text{S/cm}$	-0.030 $\mu\text{S/cm}$	2.00	0.68 $\mu\text{S/cm}$
1413.0 $\mu\text{S/cm}$	1414 $\mu\text{S/cm}$	-1.0 $\mu\text{S/cm}$	2.00	11 $\mu\text{S/cm}$
12.880 $\text{mS/cm}$	12.86 $\text{mS/cm}$	0.020 $\text{mS/cm}$	2.00	0.098 $\text{mS/cm}$

The End of Certificate

## ใบตรวจสอบสภาพเครื่องวัดสิ่งแวดล้อม

เลขที่ใบงาน: WO-00012682

ชนิดเครื่องมือ: CONDUCTIVITY METER

รุ่น: ORION STAR A215

หมายเลขเครื่อง: X58031

ตรวจสอบ (รับ)		รายการตรวจเช็ค	ตรวจสอบ (ส่ง)		หมายเหตุ
25 Dec 2023			25 Dec 2023		
ปกติ	ไม่ปกติ		ปกติ	ไม่ปกติ	
		General			
<input checked="" type="checkbox"/>	<input type="checkbox"/>	1. ความสมบูรณ์เครื่อง	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	2. ความสะอาด ( ช่องใส่ตัวอย่าง, ภายใน-นอกเครื่อง)	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	3. สวิตช์ ปิด – เปิด เครื่อง (On-Off Swich)	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	4. ปุ่มกด (Keypad)	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	5. หน้าจอ (Display, Screen Contrast)	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
		Spectrophotometer			
<input type="checkbox"/>	<input type="checkbox"/>	6. แรงดันไฟฟ้า (Battery Backup) >= 2.5 VDC	<input type="checkbox"/>	<input type="checkbox"/>	
<input type="checkbox"/>	<input type="checkbox"/>	7. ตัวหมุนเลือกความยาวคลื่น (Wavelength Control)	<input type="checkbox"/>	<input type="checkbox"/>	
<input type="checkbox"/>	<input type="checkbox"/>	8. ความยาวคลื่น (Wavelength Check)	<input type="checkbox"/>	<input type="checkbox"/>	
<input type="checkbox"/>	<input type="checkbox"/>	9. แหล่งกำเนิดแสง (UV < 3,000 hour)	<input type="checkbox"/>	<input type="checkbox"/>	
<input type="checkbox"/>	<input type="checkbox"/>	10. แหล่งกำเนิดแสง (Visible < 5,000 hour)	<input type="checkbox"/>	<input type="checkbox"/>	
<input type="checkbox"/>	<input type="checkbox"/>	11. ช่องวัดหลายตัวอย่าง (Carousel Module)	<input type="checkbox"/>	<input type="checkbox"/>	
		pH Meter and Conductivity Meter			
<input checked="" type="checkbox"/>	<input type="checkbox"/>	12. อิเล็กโทรด ( Electrode and Connection Cable )	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input type="checkbox"/>	<input type="checkbox"/>	13. ระดับสารละลายใน Electrode (Level KCl )	<input type="checkbox"/>	<input type="checkbox"/>	
<input type="checkbox"/>	<input type="checkbox"/>	14. ฝาปิดกันปลาย Electrode (Dust Protection Hood)	<input type="checkbox"/>	<input type="checkbox"/>	
<input type="checkbox"/>	<input type="checkbox"/>	15. ขาจับอิเล็กโทรด (Stand)	<input type="checkbox"/>	<input type="checkbox"/>	
		Turbidimeter			
<input type="checkbox"/>	<input type="checkbox"/>	16. ค่าความขุ่นที่ต่ำสุด (No Sample)	<input type="checkbox"/>	<input type="checkbox"/>	
<input type="checkbox"/>	<input type="checkbox"/>	17. ระดับการส่องสว่างของแสง (>= 2.5 ไม่เกิน 3.0)	<input type="checkbox"/>	<input type="checkbox"/>	
		Automatic titrator			
<input type="checkbox"/>	<input type="checkbox"/>	18. สภาพ Piston Burettes	<input type="checkbox"/>	<input type="checkbox"/>	
<input type="checkbox"/>	<input type="checkbox"/>	19. Function Rinsing and Dosing	<input type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	20. ระบบท่อสายยางและอุปกรณ์ประกอบ	<input type="checkbox"/>	<input type="checkbox"/>	

ข้อเสนอแนะ :

Mr.Siwapan Srijan

Service Engineer

บริษัท ดีเคเอสเอช เทคโนโลยี จำกัด

DKSH Technology Limited

2533 ถนนสุขุมวิท แขวงบางจาก เขตพระโขนง กรุงเทพมหานคร 10260

2533 Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260

Phone: +66 2639 7000 Email: info.calibration@dksh.com Website: www.dksh.com/scientific-thailand

Delivering Growth – in Asia and Beyond.

CAL-FM-R31-03; 20 Jul 2022



**TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)**  
**CORPORATE SERVICES 3 : EQUIPMENT CALIBRATION AND TESTING SERVICES**

534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250

TEL. 0-2717-3000 FAX. 0-2719-9484

**Cert.No.:** 24TW127

**Page.:** 1 of 2

## Certificate of Testing

**Equipment :** DO Meter  
**Manufacturer :** Mettler Toledo  
**Model :** Seven2Go Pro  
**Serial No. :** B619449111  
**ID No. :** CHM\_LG0002  
**Received Date :** 18 June 2024  
**Test Date :** 19 June 2024  
**Reference :** 2406-0561DSC-1  
**Submitted by :**

ALS Laboratory Group (Thailand) Co.,Ltd.  
104 Phatthanakan 40, Phatthanakan Rd.,  
Khwaeng Phatthanakan, Khet Suan Luang,  
Bangkok 10250 Thailand

**Laboratory Condition :**

Temperature (  $25 \pm 5$  ) °C

Humidity (  $50 \pm 20$  ) %

**Test Procedure :**

In - house method : CP-CH9

by Comparison Technique with Azide Modification Method

**Tested by :**

Walalak Sirithean

**Approved by :**

*Saithip*  
Approved Signatory

( ) Unnopphol Harachai

( ) Ponpan Paipim

(✓) Saithip Meangmai

**Issue Date :**

20 June 2024

REVIEW BY	<i>Chayathron P.</i>
APPROVED BY	<i>J. Varakorn P.</i>
NEXT CAL DATE	19/06/25



**Cert.No.:** 24TW127

**Page.:** 2 of 2

**Condition of this result of calibration**

**1. Reference Standard Instruments :**

This certification is traceable to the International System of Unit through the reference standards laboratory of Industrial Calibration Center, Technology Promotion Association (Thailand-Japan).

<b><u>Instruments</u></b>	<b><u>Serial No.</u></b>	<b><u>ID No.</u></b>	<b><u>Certificate No.</u></b>	<b><u>Due Date</u></b>
1. Burette	-	130BU10	23CG1172	22 Mar 2025
2. Balance	14233821	110RC001	23MM405	16 July 2024

**2. Standard Material :-**

<b><u>Material</u></b>	<b><u>Manufacturer</u></b>	<b><u>Lot.No.</u></b>	<b><u>Assay</u></b>
Sodium Thiosulfate pentahydrate	Merck	AM1763316	100.2%

**Result :**      **Dissolved Oxygen Meter Adjustment With Air 100 %**

**Dissolved Oxygen Probe No.:**      497482

<b>Titration Method (Azide Modification Method) (mg/L)</b>	<b>DO Meter Reading (mg/L)</b>	<b>Standard Deviation (mg/L)</b>
8.10	8.14	0.0071

This report was certified only for the instrument we tested. It is allowable to use for study  
Intend to use for advertising and referral purpose is prohibited. This report may not be reproduced  
other in full, without written approval of the laboratory

-o0o-



**TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)**  
**CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES**  
 534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250  
 TEL.0-2717-3000-29 FAX.0-2719-9484



# Certificate of Calibration

**Cert. No.:** 24LM103

Page.: 1 of 2

**Equipment :** DO Meter with Sensor

**Manufacturer :** Mettler Toledo

**Model :** Seven2Go Pro

**Serial No. :** B619449111

**ID No. :** CHM\_LG0002

**Submitted by :** ALS Laboratory Group (Thailand) Co.,Ltd.  
104 Phatthanakan 40, Phatthanakan Rd.,  
Khwaeng Phatthanakan, Khet Suan Luang,  
Bangkok 10250 Thailand

**Location :** TPA On Site Calibration Laboratory

**Received Order :** 18 June 2024

**Calibrated Date :** 21 June 2024

**Ambient Temperature :** ( 26 ± 10 ) °C

**Relative Humidity :** ( 50 ± 30 ) %

**AC Line Voltage :** ( 220 ± 22 ) V

**Calibrated by :** Warakorn Lernagtrakul

**Approved by :** Kunchit  
Approved Signatory

( ) Ponpan Paipim  
( ) Suwit Imjai  
(✓) Kunchit Promprat

**Issue Date :** 24 June 2024

**The Uncertainties are for a confidence probability of approximately 95%**

This certificate may not be reproduced other than in full, except with the prior written Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.



**Equipment :** DO Meter with Sensor  
**Condition As-Received :** Used Item  
**Reference :** 2406-0561DSC-2

**Cert. No.:** 24LM103

**Page.:** 2 of 2

**Procedure Used :-**

Calibration were conducted using in-house calibration procedure CP-OT01 according to comparison with Industrial Platinum Resistance Thermometer ( IPRT ) into Temperature Bath.

The temperature scale used was based on ITS-90.

**Condition of this result of calibration**

1. Reference standard instrument:-

<u>Instrument</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Traceable</u>	<u>Due Date</u>
1) Digital Thermometer	2188080	231216	TPA	11 Oct 2024

2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certification is traceable to the International System of Unit.

**Remark :** TPA : Technology Promotion Association ( Thailand - Japan )

**Result of Calibration :-** ( \* ) Without Adjustment

**Function :** Temperature measurement.

This instrument was connected with temperature sensor, S/N.: 497482

<u>Calibration Point</u> ( °C )	<u>Immersion Depth</u> ( mm )	<u>Standard Temperature</u> ( °C )	<u>UUC* Reading</u> ( °C )	<u>Error</u> ( °C )	<u>Uncertainty</u> ( ± °C )	<u>Coverage Factor</u> <i>k</i>
20.0	90	20.002	20.1	0.098	0.16	2.00

**UUC\* :** Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

Sartorius (Thailand) Co., Ltd.  
129 Rama 9 Road, Huaykwang, Huaykwang, Bangkok 10310  
Tel: +66 2643 8361-6, e-mail: service.thailand@sartorius.com



NSC-TIS-TIS 17025  
CALIBRATION 0426

SARTORIUS

REVIEW BY

finda k

APPROVED BY

Siriluk P

NEXT CAL DATE 02/08/25

Certificate

of Calibration

Model Number : MSE224S-100-DU  
Description : Analytical Balance  
Serial Number : 0027405555  
ID No. : BKK\_EN0003  
Manufacturer : Sartorius  
Certificate No. : 24BCI0270  
Issued Date : Monday, August 05, 2024  
Reference No. : 240942  
Page No. : 1 of 2

Customer Name : ALS Laboratory Group (Thailand)Co., Ltd.  
104 Phatthanakan 40,Phatthanakan Rd., Khwaeng Suan Luang, Khet Suan Luang, Bangkok 10250.

Calibrated Place : Lab Room

Calibrated By : Mr.Chonchai Inthana  
Calibration Date : Friday, August 02, 2024

Calibration  
Procedure No. : This calibration was conducted by  
Using in-house calibration procedure number (WI-003)  
Based on UKAS LAB 14 : 2019

Metrological data :

Capacity : 220 g Readability : 0.0001 g

Ambients Conditions:

Temperature : 23.0 °C ± 5.0 °C  
Humidity : 55.0 % RH ± 10.0 % RH  
Pressure : ±

Reasons for calibration

☐ New Installation ☐ Service / Repaired ☒ Re-calibration/ Maintenance

Equipment Condition: ☒ Good Operate ☐ Fair

Measurement Method UKAS Publication Ref :Lab 14

The measurement uncertainty stated is the expended uncertainty which is obtained from the standard uncertainty multiplied by the coverage factor (k=2) to provide a level of confidence of approximately 95%. It is determined in accordance with the Guide to Expression of Uncertainty in Measurement (GUM). The calibration certificate documents the traceability to National Standards, which realise the unit of measurement according to the International Standard System of Units (SI). Report of Tolerance came form list of Sartorius Metrological Specifications.

Traceability:

Model Number	Description	Traceability	Certificate No.	Due Date
YCS011-522-00	Sartorius weight set 1mg - 5000g E2,YCS011-522-00	TCS	M2308197S	23-Aug-2025
Testo 174 H	Thermo-Hygrometer , Testo 174H	ENTECH	H/T 661303,H661140	12-Nov-2024

This certificate relate and apply this equipment only.

This certificate may not be reproduced other than in full except with the prior written approval of the Verification Operation Division Sartorius (Thailand) Co., Ltd.

Chonchai Inthana

Mr.chonchai Inthana(Technical Manager)

S  
T  
A  
M  
P



**Sartorius (Thailand) Co., Ltd.**

129 Rama 9 Road, Huaykwang, Huaykwang, Bangkok 10310

Tel: +66 2643 8361-6 Fax: +66 2643-8367, e-mail: service.thailand@sartorius.com

**SARTORIUS**

# Certificate of Calibration

Model Number : MSE224S-100-DU

Certificate No. : 24BCI0270

Description : Analytical Balance

Issued Date : Monday, August 05, 2024

Serial Number : 0027405555

Reference No. : 240942

ID No. : BKK\_EN0003

Manufacturer : Sartorius

Page No. : 2 of 2

## Calibration Results : Without Adjustment

### Repeatability



The reproducibility is the ability of a weighing instrument to display nearly identical readouts under constant test conditions when the same load within a measurement series is placed repeatedly on the weighing pan in the same manner. The standard deviation is used to express reproducibility quantitatively.

Nominal Value : (Low Load)	20.0000	200.0000
20 g	20.0000	199.9999
Tolerance	20.0001	200.0000
0.0001 g	20.0000	200.0000
Nominal Value : (High Load)	20.0000	200.0000
200 g	20.0001	200.0001
Tolerance	20.0000	200.0000
0.0001 g	20.0000	199.9999
	20.0000	200.0000
Standard Deviation	0.000004	0.000006

### Eccentricity (Off-center loading error)

The off-center loading error is yielded by the difference between the readout of the load, i.e. 1/3 or 1/4 of maximum capacity, placed in the middle of the weighing pan and between each of four additional measurement points (positions defined according to OIML R76).

Nominal value : 100 g  
Tolerance 0.0004 g



	Difference
1	-
2	0.0000
3	0.0000
4	0.0000
5	0.0001
6	-

### Linearity

The linearity, also called linearity error. Describes the deviation of the characteristic curve of a weighing instrument from the linear slope.

Tolerance 0.0002 g

Nominal Value (g)	Conventional Mass Value (g)	Displayed Value (g)	Deviation (g)	Uncertainty (g)
0.01	0.0100	0.0100	0.0000	0.00015
0.1	0.1000	0.1000	0.0000	0.00015
1	1.0000	1.0000	0.0000	0.00015
2	2.0000	2.0000	0.0000	0.00015
5	5.0000	5.0000	0.0000	0.00015
10	10.0000	10.0000	0.0000	0.00015
20	20.0000	20.0000	0.0000	0.00015
50	50.0000	50.0001	0.0001	0.00016
100	100.0000	100.0001	0.0001	0.00019
200	200.0000	200.0000	0.0000	0.00029

End of Report.



# Metrological Center

## SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110, Thailand.

Saraburi Tel : +66 3627 3096 Fax : +66 3627 3100

Bangkok Tel : +668 9205 6851 , +669 8247 2360

Website : www.scieco.co.th E-Mail : calibrate@scg.com



Certificate No. T231303

Page 1 of 3

## Certificate of Calibration

Equipment : Liquid Bath ( Water )

Manufacturer : MEMMERT

Model : WNB29

Serial No. : L611.0135

Customer Code : BKK\_EN0148

ID No. : T6455A4

Customer : ALS Laboratory Group (Thailand) Co.,Ltd.

104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan,

Khet Suan Luang, Bangkok 10250

Customer Location : ORGANIC PREPARATION LAB

Date of Receipt : 27 June 2023

Calibrated By : Sujjar Naknakred ( Site Calibration Manager )

Approved By : Boonchai Suriyawong / Boonchai Suriyawong (Site Calibration Manager)

Date of Issue : 11 JUL 2023

REVIEW BY	<u>Siriluk P.</u>
APPROVED BY	<u>KL AL</u>
NEXT CAL. DATE	<u>04/01/25</u>

The uncertainties are for a confidence probability of approximately 95%.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standard laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Metrological Center.

Certificate No. T231303

Page 2 of 3

## Calibration Report

**Equipment** : Liquid Bath ( Water )  
**Date of Calibration** : 4 July 2023  
**Environment** : Temperature : 22.2-22.5 °C  
Line Voltage : 221.6-224.8 V  
Relative Humidity : 55 - 65 %RH

### Condition of this results of calibration :

1. This equipment was calibrated by insert five resistance thermometer detectors into its water bath , the other one thermocouple type T use for ambient temperature measurement . The calibration was done in according to WI-T36 ( based on ASTM E715-80 ( Reapproved 2001 ) ).

All data show below were final values and the initial data from customer request . The temperature scale used was based on ITS - 90 .

2. Reference Standard Instrument :

Instrument	Model	Instrument No.	Certificate No.	Due Date
RTD	100 OHM	M18 (CH1,CH6-CH7,CH9-CH10)	T230545	10 April 2024
DATA LOGGER	34970A	T149	T230545	10 April 2024

3. This certificate is traceable to :

National Institute of Metrology ( Thailand ) through Metrological Center ( NSC-TISI-TIS 17025 CALIBRATION 0244.)

4. Condition of calibrated item : good

Equipment Description :

Time Constant 3 Hour 45 Minute At 60 °C

5. Adjustment :

( X ) without adjustment

( ) after adjustment


Approved By. \_\_\_\_\_



Certificate No. T231303

Page 3 of 3

## Calibration Report

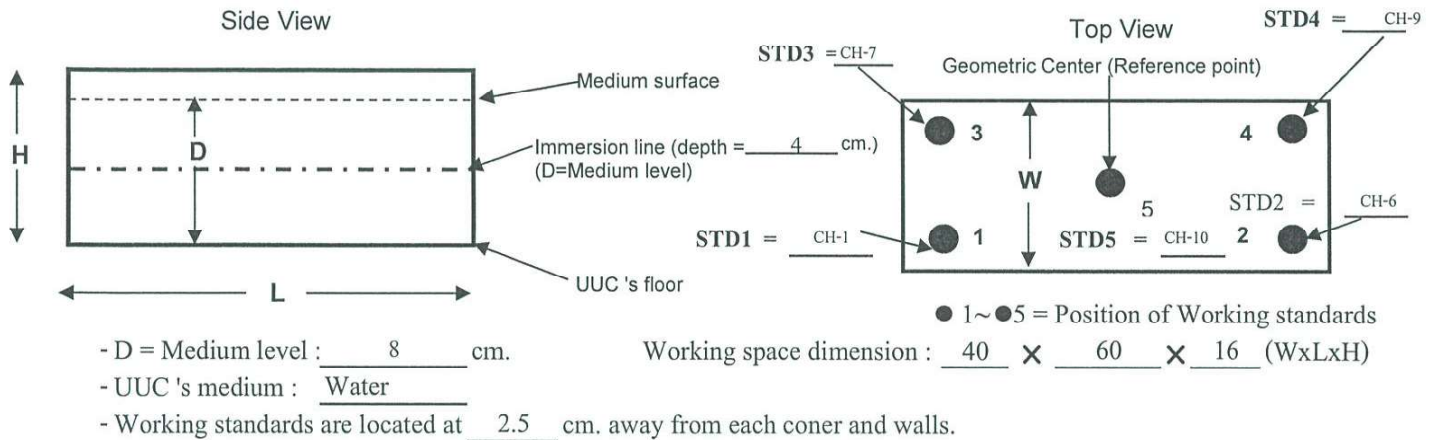

### Measurement Results:

Calibration Point	Average Standard Reading at each position (°C)				
	CH-1	CH-6	CH-7	CH-9	CH-10
60	60.03	60.06	60.24	60.11	60.18
85	84.79	84.83	85.42	85.05	85.20
95	93.71	93.83	94.62	94.15	94.42


Liquid Bath ( Water )			Temperature Distribution				
Setting (°C)	Reading (°C)		Average (°C)	Stability (± °C)	Uniformity (± °C)	Uncertainty (± °C)	Coverage Factor <i>k</i>
	Min , Max	Average					
61.0	60.9 , 61.1	61.0	60.12	0.13	0.19	0.29	2.04
86.0	85.8 , 86.2	86.0	85.06	0.19	0.47	0.44	2.17
95.0	94.6 , 95	94.9	94.15	0.32	0.65	0.55	2.13

\* The quoted uncertainty exclude "uniformity"

The calibration result apply only the above calibrated item.

The result of test was found accurate as shown on date and place of test only.

The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor *k* which for a t-distribution, providing a level of confidence of approximately 95 % .

Approved By. 



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)  
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES  
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250  
TEL.0-2717-3000-29 FAX.0-2719-9484



## Certificate of Calibration

Cert.No.: 24CH1295

Page.: 1 of 3

Equipment : pH Meter  
Manufacturer : Hach  
Model : HQ411d  
Serial No. : 200100031163  
ID No. : BKK\_EN0342  
Condition As-Received: Used Item  
Received Date : 16 October 2024  
Calibration Date : 17 October 2024  
Reference : 2410-0548DSC-5  
Submitted by :

REVIEW BY *Jinda K.*

APPROVED BY *Siriluk P.*

NEXT CAL DATE **17/10/25**

ALS Laboratory Group (Thailand) Co.,Ltd.  
104 Phatthanakan 40, Phatthanakan Rd.,  
Khwaeng Phatthanakan, Khet Suan Luang,  
Bangkok 10250 Thailand

Ambient Temperature : (25 ± 2.5) °C  
Relative Humidity : (50 ± 15) %  
Calibration Procedure : In - house method :  
- CP-CH5 by direct measurement with  
certified reference material (CRM)  
- CP-CH8 by comparison with temperature standard

Calibrated by : Warakorn Lerngatrakul

Approved by :

*Saithip*

Approved Signatory

- ( ) Unnopphol Harachai  
( ) Ponpan Paipim  
(✓) Saithip Meangmai

Issue Date : 21 October 2024

**The Uncertainties are for a confidence probability of approximately 95%**

This certificate may not be reproduced other than in full, except with the prior written  
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.



Cert.No.: 24CH1295

Page.: 2 of 3

**Condition of this calibration result**

1. Reference Standard Instrument

<u>Instrument</u>	<u>Serial No.</u>	<u>ID No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
1)Ref. Standard Thermometer	2188080	130RC044	2411022	16 Sep 2025

- This Certification is traceable to SI Through Technology Promotion Association (Thailand - Japan)

2. Certified Reference Materials :The measurement results are traceable to SI through Hach Lenge GmbH Ltd.

Deutsche Akkreditierungsstelle, Accredited No.D-RM-15184-01-00

:The measurement results are traceable to SI through CPA chem Ltd.,

ANSI-ASQ National Accreditation Board, Accredited No. AR-1835

<u>Buffer Solution</u>	<u>Manufacturer</u>	<u>Lot No.</u>	<u>Exp. date</u>
pH 4.008	CPA chem	1034203	27 Sep 2026
pH 6.999	Hach Lenge GmbH	C03145	28 Feb 2026
pH 10.010	CPA chem	1034205	27 Sep 2025

3. This certificate is valid only to the item calibrated on date and place of calibration.

**Calibration Results**

**Function : pH Measurement**

Performing three buffers standard curve by using buffer nominal pH (4,7,10)

<u>Unit Under Calibration</u>	<u>Standard pH Buffer Solution</u>	<u>Actual pH Reading</u>	<u>Actual mV Reading (mV)</u>	<u>Uncertainty of pH Measurement (±)</u>	<u>Coverage factor k</u>
pH Electrode S/N.: 230473042902	4.008	4.028	174.6	0.0044	2.00
	6.999	7.014	1.4	0.0084	2.05
	10.010	10.018	-172.8	0.0066	2.00

**Remark** - Can not connect the BNC because the plug does not match with the socket.



Cert.No.: 24CH1295

Page.: 3 of 3

### Calibration Results

**Function : Temperature Measurement**

**( \* ) Without adjustment**

This equipment was connected with Temperature Probe;

- Model : PHC281

- Serial No. : 230473042902

Dimension of probe

- Length : 103 mm.

- Diameter : 12 mm.


- Immersion Depth : 90 mm.

Calibration Point ( °C )	Standard Temperature ( °C )	UUC* Reading ( °C )	Error ( °C )	Uncertainty of measurement ( ± °C )	Coverage factor <i>k</i>
25.0	25.002	25.0	-0.002	0.13	2.00

**Remark : UUC\* = Unit Under Calibration**

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-



บริษัท ดับเบิล เอส ไดแอกโนสติกส์ จำกัด  
DOUBLE S DIAGNOSTICS CO., LTD.

4 ซอยอุดมสุข 14 แขวงบางนา เขตบางนา กรุงเทพฯ 10260 โทรศัพท์: (02) 747-7009 โทรสาร: (02) 747-7008  
4 Soi Udomsuk 14, Bangna, Bangkok 10260 Tel. (02) 747-7009 Fax: (02) 747-7008

Maintenance Plan YEAR : 2024

เดือน	Jan	Feb	Mar	Apr	May	Jun	Jul	Aug	Sep	Oct	Nov	Dec
รวม								6M				

Periodical maintenance check list for Konelab

	6M	12M	Note!
1.Diluent-wash tubing change	<input type="checkbox"/>	<input checked="" type="checkbox"/>	
2.ISE tubing change	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	None.
3.Syringe check/change		<input checked="" type="checkbox"/>	
4.Dispensing check/ change		<input checked="" type="checkbox"/>	
5.Waste tubing change when necessary		<input checked="" type="checkbox"/>	
6.Lamp check/change	<input type="checkbox"/>	<input checked="" type="checkbox"/>	
7.Mixer paddle/paddle change(not Konelab20)		<input checked="" type="checkbox"/>	
8.ISE needles check/change		<input checked="" type="checkbox"/>	None.
9.Pump tubing check/ chance	<input type="checkbox"/>	<input checked="" type="checkbox"/>	
10.Broken/worn out part check /change		<input checked="" type="checkbox"/>	
11.Peristaltic pump check /cleaning/ lubrication	<input type="checkbox"/>	<input checked="" type="checkbox"/>	
12.Heating check		<input checked="" type="checkbox"/>	
13.Cooling check		<input checked="" type="checkbox"/>	
14.Dispenser mechanic check/adjustment	<input type="checkbox"/>	<input checked="" type="checkbox"/>	
15.Cuvette transfer mechanic check/adjustment	<input type="checkbox"/>	<input checked="" type="checkbox"/>	
16.Dispenser movement check/adjustment	<input type="checkbox"/>	<input checked="" type="checkbox"/>	
17.Sample/reagent register check/adjustment	<input type="checkbox"/>	<input checked="" type="checkbox"/>	
18.Dispensing tubing tightness check	<input type="checkbox"/>	<input checked="" type="checkbox"/>	
19.Photometer and optics cleaning/check/adjustment	<input type="checkbox"/>	<input checked="" type="checkbox"/>	
20.Workstation PC cleaning if necessary	<input type="checkbox"/>	<input checked="" type="checkbox"/>	
21.Mechanic cleaning/lubrication	<input type="checkbox"/>	<input checked="" type="checkbox"/>	
22.Instrument cleaning if necessary	<input type="checkbox"/>	<input checked="" type="checkbox"/>	
23.Complete analyzer testing with waterblank/QC or sample	<input type="checkbox"/>	<input checked="" type="checkbox"/>	
24.Test parameters/Adjustment/config. Save to USB key	<input type="checkbox"/>	<input checked="" type="checkbox"/>	
25.UPS Test	<input type="checkbox"/>	<input checked="" type="checkbox"/>	

Place: ALS LAB Instrument: K20 Aquakem  
Date/Time: 16/8/62 Serial no: 22781  
Service done by: [Signature] Install date:  
Signature of customer: [Signature] Date/Time: 16/08/2024

Laboratory  
Analyzer User

8/16/2024 14:53

Performed                      8/16/2024  
Lot                              WB34

# ACCEPTANCE CRITERIA

	Result	Limit	Warning
Temperature (?C)	37.8	37.0 +/- 1.0	
Dispensing ratio	16.4	14.8 - 17.2	
CV%	0.29	<1.7	
Photometric noise			
Max SD L340_2 (mA)	0.17	<2.0	
Max SD L340_4 (mA)	0.87	<3.0	
Linearity of photometer			
Slope	1.0141	0.94 - 1.06	
Curvature	0.0053	+/- 0.02	
Max bias from linear fit (mA)	4.3	<15.0	
Max delta %	-1.6	+/- 6.0	
Linearity of sample dispensing			
Proport. volume XDISP2 (?l)	2.06	1.96 - 2.16	
Proport. volume XDISP4 (?l)	4.14	3.85 - 4.40	
XDISP2 CV%	1.21	<2.0	
XDISP4 CV%	0.90	<2.0	
XDISP10 CV%	0.68	<2.0	
Needle 0 ?l volume			
Average (A)	0.005	<0.050	
Standard deviation (A)	0.002	<0.005	
Volume (?l)	0.03	<0.32	

# OTHER INFORMATION

Dispensing ratio		Photom. noise: SD (mA)	
Posit	Result (A)	Posit	L340_2      L340_4
1	0.1549	1	0.15      0.80
2	0.1549	2	0.17      0.79
3	0.1537	3	0.04      0.65
4	0.1547	4	0.16      0.31
5	0.1547	5	0.11      0.58
6	0.1545	6	0.14      0.87

Laboratory  
Analyzer User


8/16/2024 14:53

Linearity of sample dispensing

Test	Absorbance (A)
XDISP2	0.306
XDISP4	0.612
XDISP10	1.471

Linearity of photometer

L340_	Target (A)	Meas (A)	Delta (A)	Delta %
1	0.002	0.006	-0.004	-217.7
2	0.486	0.493	-0.007	-1.5
3	1.451	1.469	-0.018	-1.2
4	1.936	1.963	-0.027	-1.4
5	2.415	2.454	-0.039	-1.6

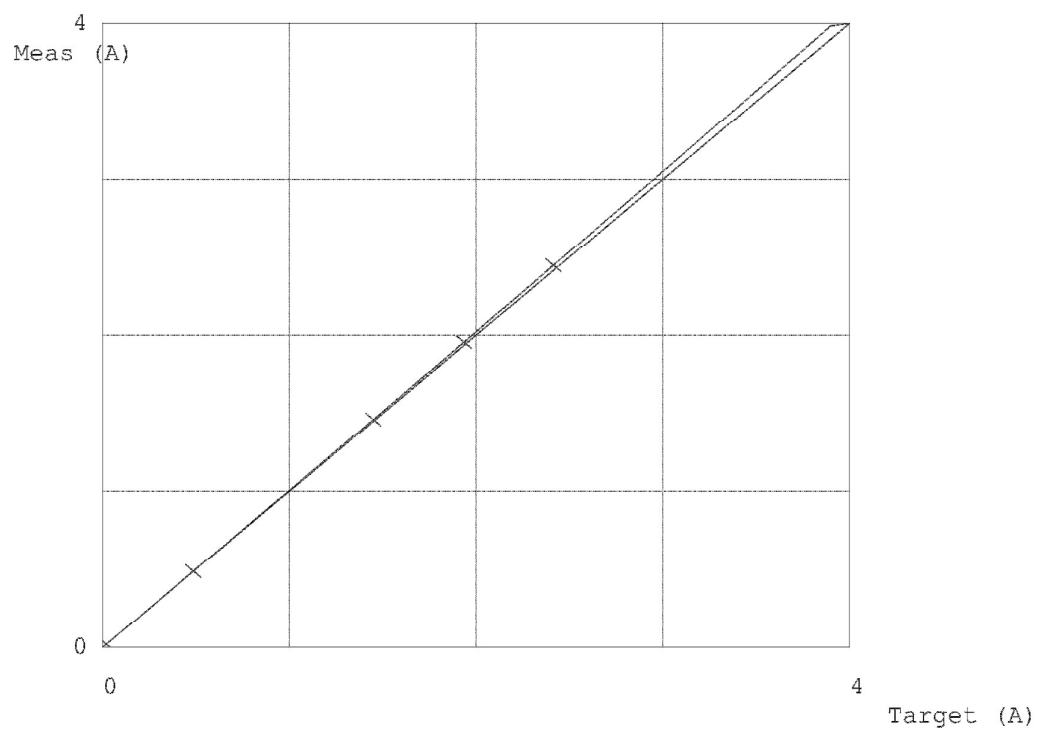



## Certificate of Calibration

Cert.No.: 24CH228

Page.: 1 of 3

Equipment :	pH Meter
Manufacturer :	Mettler Toledo
Model :	Seven2Go pH/mv S2
Serial No. :	B626673720
ID No. :	CHM_LG0001
Condition As-Received:	Used Item
Received Date :	16 February 2024
Calibration Date :	19 February 2024
Reference :	2402-0552DSC-1
Submitted by :	ALS Laboratory Group (Thailand) Co.,Ltd. 104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan, Khet Suan Luang, Bangkok 10250 Thailand
Ambient Temperature :	(25 ± 2.5) °C
Relative Humidity :	(50 ± 15) %
Calibration Procedure :	In - house method : - CP-CH5 by direct measurement with standard voltage and direct measurement with certified reference material (CRM) - CP-CH8 by comparison with temperature standard
Calibrated by :	Warakorn Lerngagtrakul
Approved by :	 Approved Signatory
( ) Pornthippa Tameyakul	
( ) Unnopphol Harachai	
(✓) Saithip Meangmai	
Issue Date :	21 February 2024

REVIEW BY	
APPROVED BY	
NEXT CAL DATE	19/02/25

**The Uncertainties are for a confidence probability of approximately 95%**

This certificate may not be reproduced other than in full, except with the prior written  
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.



Cert.No.: 24CH228

Page.: 2 of 3

**Condition of this calibration result**

1. Reference Standard Instrument

<u>Instrument</u>	<u>Serial No.</u>	<u>ID No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
1) Document Process Calibrator	54030049	130RC116	23E2802	27 Aug 2024
2) Ref. Standard Thermometer	4982054	110RC044	23I908	26 July 2024

This certification is traceable to the International System of Unit maintained through:-

- Technology Promotion Association (Thailand-Japan)

2. Certified Reference Materials : The measurement results are traceable to SI through CPA chem Ltd.,  
ANSI-ASQ National Accreditation Board, Accredited No. AR-1835

<u>Buffer Solution</u>	<u>Manufacturer</u>	<u>Lot No.</u>	<u>Exp. date</u>
pH 4.008	CPA chem	940102	27 Nov 2025
pH 6.986	CPA chem	940104	02 Nov 2024
pH 9.997	CPA chem	940106	02 Nov 2024

3. This certificate is valid only to the item calibrated on date and place of calibration.

**Calibration Results**

**Function : mV Measurement**

**Performing standard curve by Document Process Calibrator at pH (4,7,10)**

Unit Under Calibration	Nominal Value	Standard Voltage Input	Actual Reading		Uncertainty of Measurement ( ±mV )	Coverage factor <i>k</i>
	pH	mV	mV	pH		
pH Meter S/N.: B626673720	4.00	177.48	177	4.00	0.58	2.00
	7.00	0.00	0	7.00	0.58	2.00
	10.00	-177.48	-178	10.00	0.58	2.00



Cert.No.: 24CH228

Page.: 3 of 3

### Calibration Results

#### Function : pH Measurement

Performing three buffers standard curve by using buffer nominal pH (4,7,10)

Unit Under Calibration	Standard pH Buffer Solution	Actual pH Reading	Actual mV Reading (mV)	Uncertainty of pH Measurement ( $\pm$ )	Coverage factor $k$
pH Electrode S/N.: 6344910	4.008	4.01	212	0.0079	2.00
	6.986	6.99	38	0.0093	2.00
	9.997	10.01	-139	0.0095	2.00

#### Function : Temperature Measurement

##### (\*) Without adjustment

This equipment was connected with Temperature Probe;

- Model : InLab®Expert Go-ISM

- Serial No. : 6344910

Dimension of probe

- Length : 120 mm.

- Diameter : 12 mm.

- Immersion Depth : 100 mm.

Calibration Point (°C)	Standard Temperature (°C)	UUC* Reading (°C)	Error (°C)	Uncertainty of measurement ( $\pm$ °C)	Coverage factor $k$
25.0	25.002	25.0	-0.002	0.13	2.00
45.0	45.002	45.1	0.098	0.13	2.00

**Remark** - UUC\* = Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor  $k$ , providing a level of confidence of approximately 95 %.

-o0o-



# Metrology

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110, Thailand.

Saraburi Tel : +66 3627 3096 Fax : +66 3627 3100

Bangkok Tel : +668 9205 6851 , +669 8247 2360

Website : www.scieco.co.th E-Mail : calibrate@scg.com



Certificate No. T240904

Page 1 of 3

## Certificate of Calibration

Equipment : Chamber ( Oven )

Manufacturer : Memmert

Model : UF 450

Serial No. : B717.0531

Customer Code : BKK\_EN0273

ID No. : T8042A4

Customer : ALS Laboratory Group (Thailand) Co.,Ltd.


104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan,

Khet Suan Luang, Bangkok 10250

Customer Location : Laboratory (Oven Room)

Date of Receipt : 08 May 2024

Calibrated By : Preecha Phisassutthikul ( Temperature Calibration Manager )

Approved By :  / Nuafun Sungchum (Metrology Manager)

Date of Issue : 23 MAY 2024

REVIEW BY	<i>Jinda K</i>
APPROVED BY	<i>Siriluk P</i>
NEXT CAL. DATE	14/11/25

The uncertainties are for a confidence probability of approximately 95%.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standard laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Metrology.

Certificate No. T240904

Page 2 of 3

## Calibration Report

**Equipment** : Chamber ( Oven )  
**Date of Calibration** : 14 May 2024  
**Environment** : Temperature : 26.5-28.1 °C  
Line Voltage : 226.7-229.8 V  
Relative Humidity : 51 - 57 %RH

### Condition of this results of calibration :

1. This equipment was calibrated by insert nine resistance thermometer detectors into its chamber , the other one resistance thermometer detector use for ambient temperature measurement . The calibration was done in according to WI-T20 ( based on ASTM E145-94 ( Reapproved 2001) and AS2853-1986 ).

All data show below were final values and the initial data from customer request . The temperature scale used was based on ITS - 90 .

2. Reference Standard Instrument :

Instrument	Model	Instrument No.	Certificate No.	Due Date
RTD	100 ohm	21-(CH1-10)	T231955	17 November 2024
DATA LOGGER	34970A	T121	T231955	17 November 2024

3. This certificate is traceable to :

National Institute of Metrology ( Thailand ) through Metrological Center ( NSC-TISI-TIS 17025 CALIBRATION 0244.)

4. Condition of calibrated item : good

Equipment Description :


Time Constant 1 Hour 30 Minute At 104 °C  
Fresh Air Damper ☐ Open ☐ Min ☐ Medium ☐ Max  
☐ Close  
☒ Not Available

5. Adjustment :


( X ) without adjustment

( ) after adjustment

Approved By \_\_\_\_\_



## Calibration Report

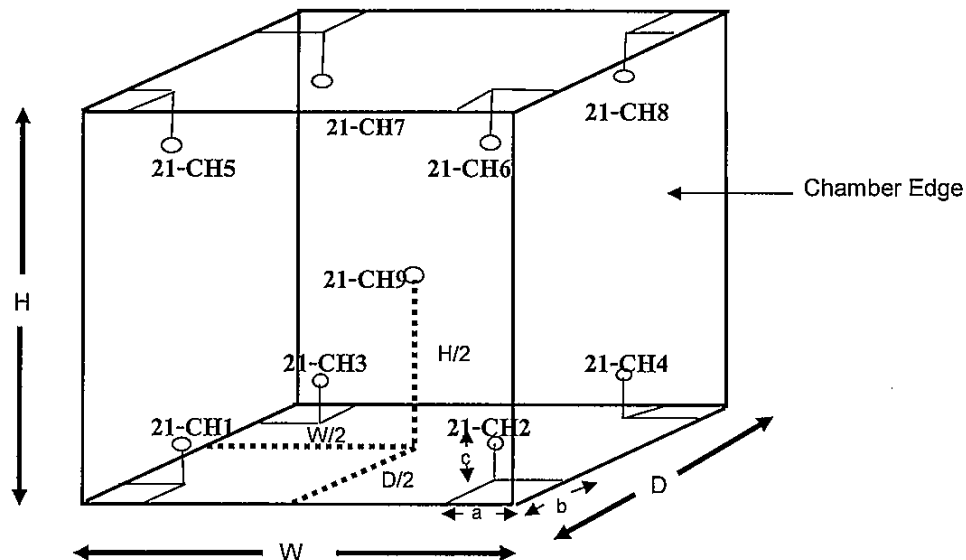

**Remark :**

Internal Dimensions of Chamber : W (Width) = 104 cm. , H(Height)=72 cm. and D(Depth)=60 cm.

Size of Installed Standard sensor number 21-CH1 to number 21-CH8 : a = 5 cm. , b = 5 cm. and c = 5 cm.

Size of Installed Standard sensor number 21-CH9 : W/2=104 cm./2 , H/2=72 cm./2 and D/2=60 cm./2

**Measurement Results**

Calibration Point	Average Standard Reading at each position (°C)								
	21-CH1	21-CH2	21-CH3	21-CH4	21-CH5	21-CH6	21-CH7	21-CH8	21-CH9
104	103.4	105.0	103.7	103.6	103.3	104.6	103.3	104.0	103.9
180	179.5	181.1	179.2	179.5	179.0	181.3	179.8	179.9	180.2

Chamber ( Oven )			Temperature Distribution				
Setting (°C)	Reading (°C)		Average (°C)	Stability (±°C)	Uniformity (°C)	Uncertainty (±°C)	Coverage Factor k
	Min , Max	Average					
104.0	103.9 , 104	104.0	103.85	0.14	1.27	0.44	2.00
180.0	179.9 , 180.1	180.0	179.94	0.39	2.29	0.76	2.00


\* The quoted uncertainty exclude "uniformity"

The calibration result apply only the above calibrated item.

The result of test was found accurate as shown on date and place of test only.

The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor  $k$  which for a t-distribution, providing a level of confidence of approximately 95 % .

End of Certificate

Approved By. 



# Metrological Center

## SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110

Telephone : +66 2 586 5792-4 Fax : +66 2 586 5109

Website : www.scieco.co.th E-Mail : calibrate@scg.co.th

Certificate No. T240742

Page 1 of 5

## Certificate of Calibration

Equipment : Digestion Unit

Manufacturer : SCP Science

Model : DigiPRER HT

Serial No. : HTC1120480658

Customer Code : BKK\_EN0366

ID No. : T2635A5

Customer : ALS Laboratory Group (Thailand) Co.,Ltd.

104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan,

Khet Suan Luang, Bangkok 10250

Customer Location : Wet Chemistry Lab 1

Date of Receipt : 11 April 2024

Calibrated By : Sujjar Naknakred ( Site Calibration Manager )

Approved By :  / Boonchai Suriyawong ( Site Calibration Manager )

Date of Issue : 02 MAY 2024

REVIEW BY	<i>Linda K.</i>
APPROVED BY	<i>Siriluk P.</i>
NEXT CAL. DATE	<i>21/04/25</i>

The uncertainties are for a confidence probability of approximately 95%.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standard laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Metrological Center.



# Metrological Center

## SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110

Telephone : +66 2 586 5792-4 Fax : +66 2 586 5109

Website : www.scieco.co.th E-Mail : calibrate@scg.co.th

Certificate No. T240742

Page 2 of 5

## Calibration Report

Equipment : Digestion Unit  
Date of Calibration : 21 April 2024  
Environment : Temperature : 23.9 - 26.3 °C  
Line Voltage : 221.8 - 225.9 V  
Relative Humidity : 55 - 65 %RH

### Condition of this results of calibration :

1. This equipment was calibrated by insert four standard thermocouples type S into its chamber , the other one thermocouple type T use for ambient temperature measurement . The calibration was done in according to WI-T10.  
was based on ITS - 90 .

### 2. Reference Standard Instrument :

Instrument	Model	Instrument No.	Certificate No.	Due Date
TC	Type S	M20A2-(CH11-CH14)	T230886	09 May 2024
DATA LOGGER	34970A	T47	T230886	09 May 2024

### 3. This certificate is traceable to :

National Institute of Metrology ( Thailand ) through Metrological Center ( NSC-TISI-TIS 17025 CALIBRATION 0244.)

### 4. Condition of calibrated item : good

Equipment Description :

Time Constant 1 Hour 6 Minute At 380 °C  
Fresh Air Damper ☐ Open ☐ Min ☐ Medium ☐ Max  
☐ Close  
☒ Not Available

### 5. Adjustment :

( X ) without adjustment


( ) after adjustment

Approved By

Certificate No. T240742

Page 3 of 5

## Calibration Report

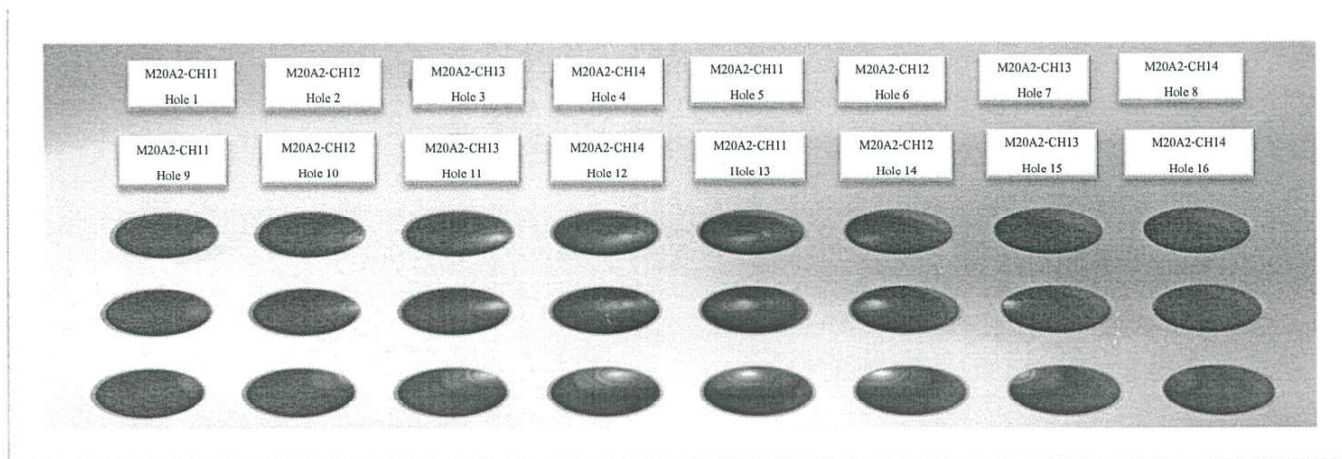

FRONT

### Measurement Results

Cal. Point	Setting	Reading	STD.	Position of Standards at Block							
(°C)	(°C)	(°C)	Reading	M20A2-CH11 Hole 1	M20A2-CH12 Hole 2	M20A2-CH13 Hole 3	M20A2-CH14 Hole 4	M20A2-CH11 Hole 5	M20A2-CH12 Hole 6	M20A2-CH13 Hole 7	M20A2-CH14 Hole 8
380.0	380.0	379.2 - 380.5	Max °C	378.7	378.9	377.9	378.7	380.5	379.8	378.7	377.4
			Min °C	378.2	378.5	377.5	378.2	380.1	379.3	378.3	376.9
			Average °C	378.4	378.7	377.7	378.4	380.3	379.6	378.5	377.2
			Stability ± °C	0.2	0.2	0.2	0.2	0.2	0.3	0.2	0.2

Cal. Point	Setting	Reading	STD.	Position of Standards at Block							
(°C)	(°C)	(°C)	Reading	M20A2-CH11 Hole 9	M20A2-CH12 Hole 10	M20A2-CH13 Hole 11	M20A2-CH14 Hole 12	M20A2-CH11 Hole 13	M20A2-CH12 Hole 14	M20A2-CH13 Hole 15	M20A2-CH14 Hole 16
380.0	380.0	379.2 - 380.5	Max °C	378.4	378.6	379.2	379.6	381.9	380.6	379.1	378.1
			Min °C	377.8	378.2	378.7	379.2	381.4	379.9	378.3	377.2
			Average °C	378.1	378.4	379.0	379.4	381.6	380.3	378.7	377.7
			Stability ± °C	0.3	0.2	0.2	0.2	0.3	0.4	0.4	0.5


Approved By. \_\_\_\_\_



Certificate No. T240742

Page 4 of 5

## Calibration Report

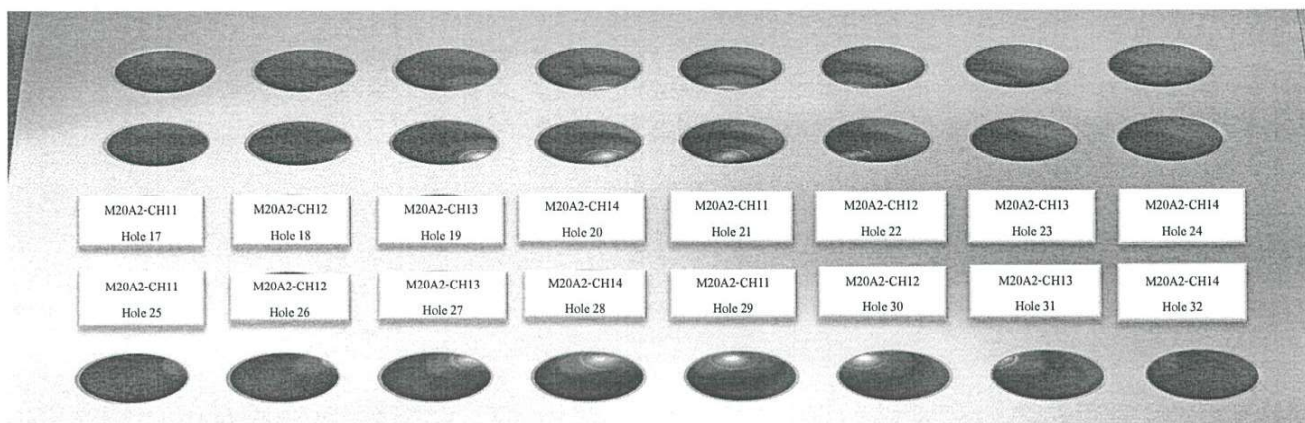

FRONT

### Measurement Results

Cal. Point	Setting	Reading	STD.	Position of Standards at Block							
(°C)	(°C)	(°C)	Reading	M20A2-CH11 Hole 17	M20A2-CH12 Hole 18	M20A2-CH13 Hole 19	M20A2-CH14 Hole 20	M20A2-CH11 Hole 21	M20A2-CH12 Hole 22	M20A2-CH13 Hole 23	M20A2-CH14 Hole 24
380.0	380.0	379.2 - 380.5	Max °C	378.9	379.2	379.5	380.1	382.1	381.0	378.9	377.8
			Min °C	378.2	378.6	379.1	379.6	381.7	380.2	378.3	377.2
			Average °C	378.5	378.9	379.3	379.8	381.9	380.6	378.6	377.5
			Stability ± °C	0.3	0.3	0.2	0.2	0.2	0.4	0.3	0.3

Cal. Point	Setting	Reading	STD.	Position of Standards at Block							
(°C)	(°C)	(°C)	Reading	M20A2-CH11 Hole 25	M20A2-CH12 Hole 26	M20A2-CH13 Hole 27	M20A2-CH14 Hole 28	M20A2-CH11 Hole 29	M20A2-CH12 Hole 30	M20A2-CH13 Hole 31	M20A2-CH14 Hole 32
380.0	380.0	379.2 - 380.5	Max °C	378.5	378.1	378.0	378.6	380.7	379.7	377.7	380.9
			Min °C	378.2	377.8	377.7	378.1	380.3	379.0	377.2	380.4
			Average °C	378.4	378.0	377.9	378.4	380.5	379.4	377.5	380.6
			Stability ± °C	0.2	0.2	0.2	0.2	0.2	0.3	0.2	0.3


Approved By. \_\_\_\_\_



Certificate No. T240742

Page 5 of 5

## Calibration Report

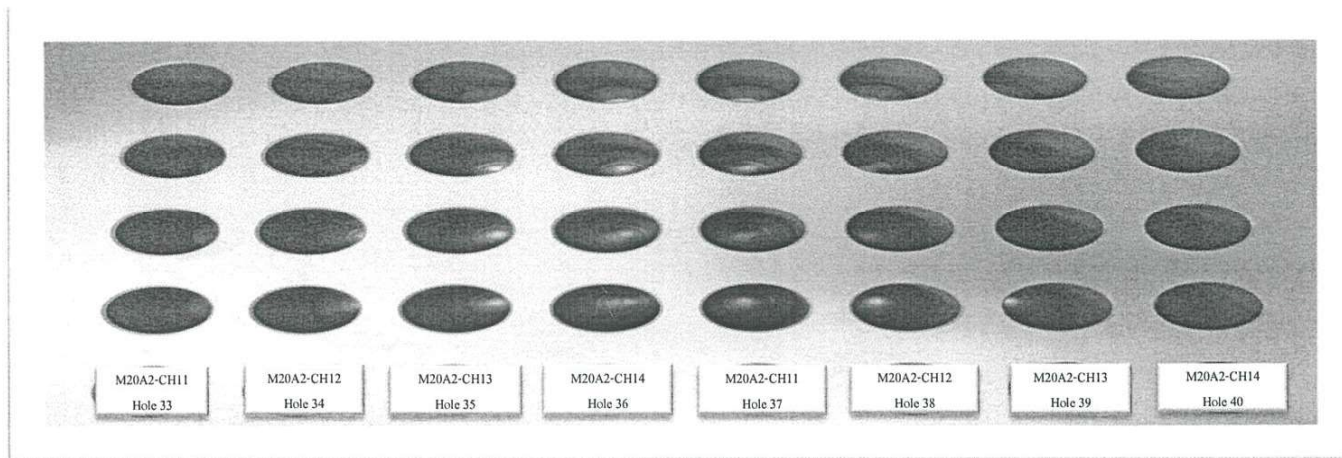

FRONT

### Measurement Results

Cal. Point	Setting	Reading	STD.	Position of Standards at Block							
(°C)	(°C)	(°C)	Reading	M20A2-CH11 Hole 33	M20A2-CH12 Hole 34	M20A2-CH13 Hole 35	M20A2-CH14 Hole 36	M20A2-CH11 Hole 37	M20A2-CH12 Hole 38	M20A2-CH13 Hole 39	M20A2-CH14 Hole 40
380.0	380.0	379.2 - 380.5	Max °C	378.3	377.9	378.7	379.5	381.6	380.5	378.4	378.0
			Min °C	378.0	377.6	378.4	379.1	381.2	380.0	378.1	377.6
			Average °C	378.2	377.8	378.6	379.3	381.4	380.3	378.2	377.8
			Stability ± °C	0.2	0.2	0.2	0.2	0.2	0.2	0.2	0.2

The expanded uncertainty of temperature measurement was  $\pm 1.87^{\circ}\text{C}$

The calibration result apply only the above calibrated item.

The result of test was found accurate as shown on date and place of test only.

The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor  $k=2$ , providing a level of confidence of approximately 95 %.

Approved By. \_\_\_\_\_






## MULTIPOINT CALIBRATION REPORT

Calibration Date 3-Jul-24  
Manufacturer HORIBA  
Serial No. XLTWBBSJ  
Calibrator Manufacturer Teledyne API  
Serial No. 947  
Std. Gas Concentration (PPM) 55.88  
Cylinder Pressure (psi) 1800  
Certified Date 9-Feb-22

Equipment Name NOx Analyzer  
Model APNA-370  
Equipment ID BKK\_FS1092  
Model 700  
Cylinder No. GN0027222  
Certified By Airgas Inc.  
Expired Date 9-Feb-30

Point	CALIBRATION RESULTS						
	Ideal	Actual NO	Error NO	%Error NO	Actual NOx	Error NOx	%Error NOx
ZERO	0.00	0.10	0.10	0.10	0.10	0.10	0.10
1	100.00	99.70	-0.30	-0.30	101.00	1.00	1.00
2	200.00	198.10	-1.90	-0.95	201.20	1.20	0.60
3	300.00	299.20	-0.80	-0.27	301.40	1.40	0.47
4	400.00	398.20	-1.80	-0.45	402.10	2.10	0.53
AVERAGE (%)				-0.37			0.54

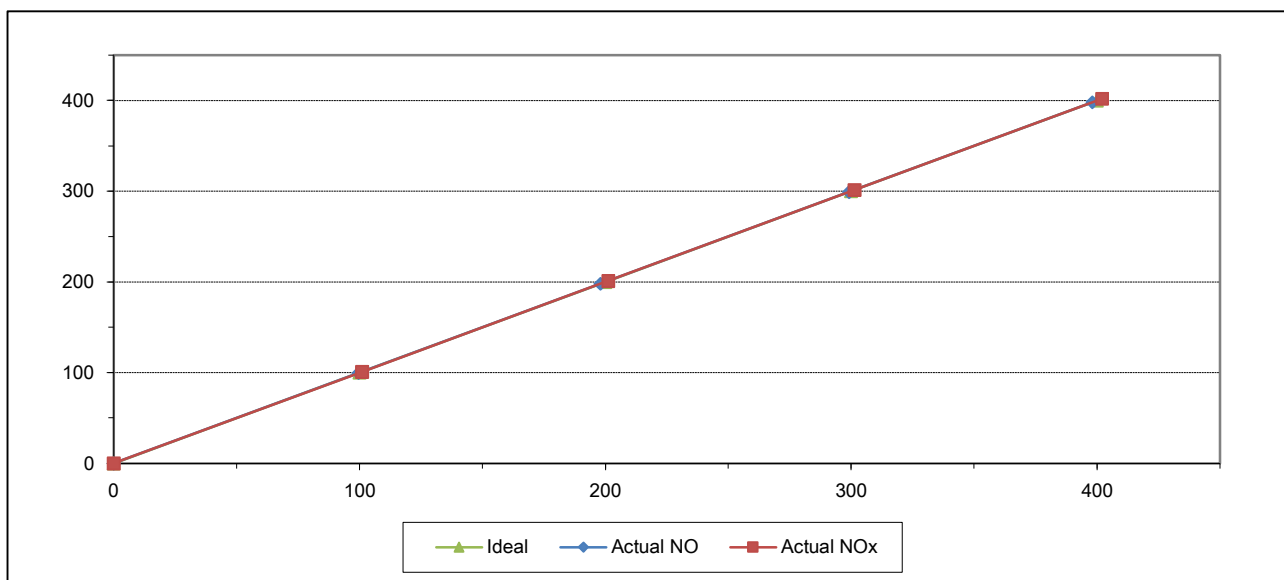

Calibrated By

( Mr.Jirawut Sakarn )  
Field Environmental Scientist (3)

Approved By


( Mr.Sarayuth Jittranont )  
Assistant General Manager



## MULTIPOINT CALIBRATION REPORT

Calibration Date	5-Jul-24	Equipment Name	SO2 Analyzer
Manufacturer	HORIBA	Model	APSA-370
Serial No.	6BVW9P1K	Equipment ID	BKK_FS1091
Calibrator Manufacturer	Teledyne API	Model	700
Serial No.	947		
Std. Gas Concentration (PPM)	56.3	Cylinder No.	GN0027222
Cylinder Pressure (psi)	1800	Certified By	Airgas Inc.
Certified Date	9-Feb-22	Expired Date	9-Feb-30

Point	CALIBRATION RESULTS			
	Ideal	Autual	Error	%Error
ZERO	0.00	0.10	0.10	0.10
1	100.00	98.50	-1.50	-1.50
2	200.00	198.00	-2.00	-1.00
3	300.00	298.70	-1.30	-0.43
4	400.00	398.50	-1.50	-0.38
AVERAGE (%)				-0.64

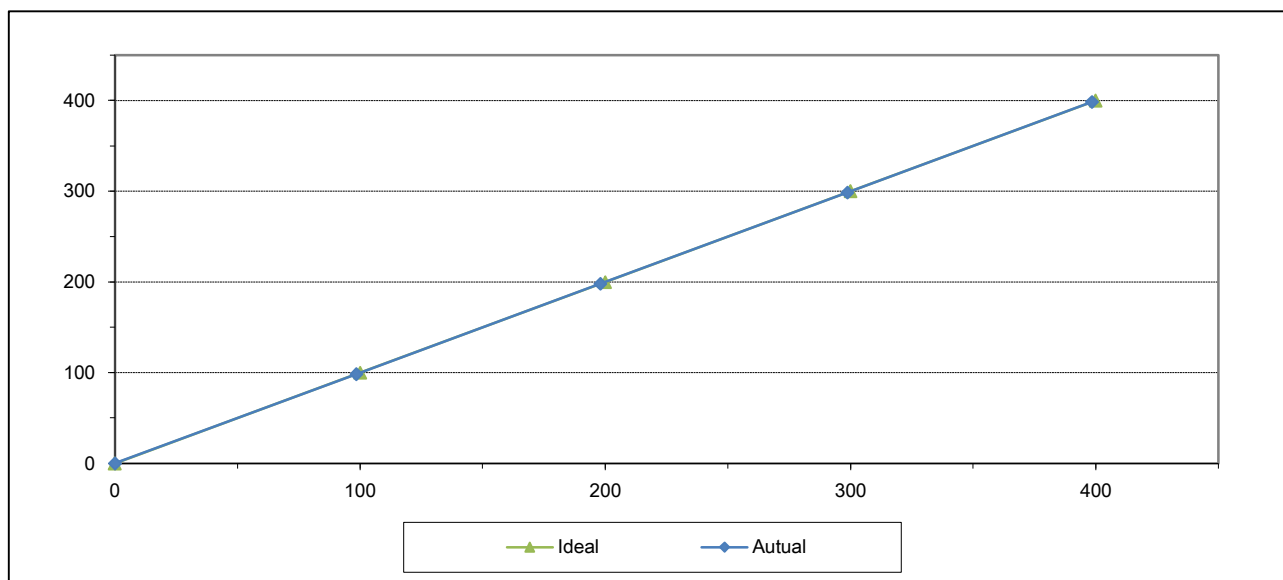

Calibrated By

( Mr.Jirawut Sakarn )  
Field Environmental Scientist (3)

Approved By


( Mr.Sarayuth Jittrantont )  
Assistant General Manager



### High Volume Air Sampler Calibration Worksheet

Project Site :	Dcondo Ping Juristic Person Condominium	Barometric Pressure (mm Hg) :	730.5
Calibrate Location :	มุมด้านหลังอาคาร C	Temperature ( °C ) :	31.5
Calibrate Date :	29-Oct-24	High Volume ID :	BKK_FS1060
CalibrationSheet No.:	C-291024-BKK_FS1060	High Volume Model :	TE-5009X
Calibrator ID:	BKK_FS0625	High Volume S/N :	5503
Calibrator Model :	TE-5028A	Calibrator Slope :	1.04803
Calibrator S/N :	2585	Calibrator Intercept :	-0.01206

Test No.	Delta H <sub>2</sub> O (inch)	Qa (m <sup>3</sup> /min)	I : Chart (CFM)	Linear Regression
1	2.4	0.966	32	Slope : 47.0957 Intercept : -13.1298 Correlation Coefficient : 0.9979
2	2.8	1.043	36	
3	3.2	1.114	40	
4	3.8	1.213	44	
5	4.4	1.304	48	

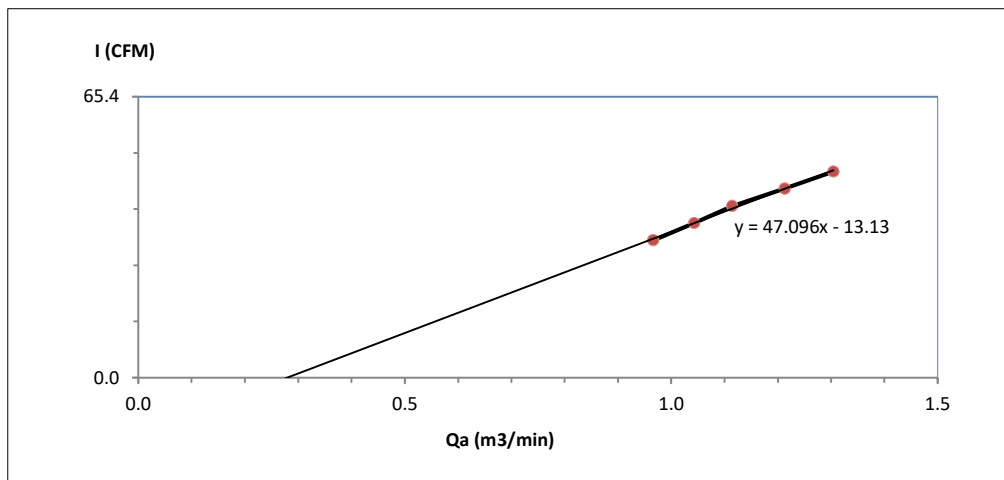

Calibrated by Jatsarawut  
( Mr.Jatsarawut Pattama )  
Field Scientist(2)

Approved by : Noppong Juntarupan  
(Mr. Noppong Juntarupan)  
Enviro Field Coordinator Scientist (3)

## CERTIFICATE OF CALIBRATION

Certificate No. : PST-0126-24

W/O No. : WO-0051-24

### Customer

Page no. 1 of 3

Company : ALS LABORATORY GROUP (THAILAND) CO., LTD.  
Address : 104 Phatthanakan 40, Phatthanakan Road, Khwaeng Phatthanakan,  
City / Province : Khet Suan Luang, Bangkok  
Zip/Postal : 10250

### Device

Equipment : Electronic Balance Capacity : 120 / 220 g  
Manufacturer : OHAUS Readability : 0.00001 / 0.0001 g  
Model : EX225D/AD ID No. : BKK\_EN0403  
Serial No. : C309774648  
Condition : Normal

### Environment Conditions

Location of Calibration : Enviroment Lab  
Ambient Temperature : 20.1 (°C) ± 3 °C  
Relative Humidity : 70.3 (%RH) ± 15 %RH  
Barometric Pressure : 1011.1 (mba) ± 10 hPa  
Comment :

REVIEW BY Linda K.  
APPROVED BY Siriluk P.  
NEXT CAL. DATE 03/06/25

Date of Receipt : June 3, 2024  
Date of Calibration : June 3, 2024  
Issue Date : June 5, 2024

Calibrated by : Mr.Kittichai Rattanatham  
Calibrator

Approved by ( Mr.Kittichai Rattanatham )  
Approved Signature

The reported measurement result relates only to the measurand and applies only at the time of measurement.

This Certificate is issued in accordance with the conditions of accreditation granted by Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and is traceability to recognize national standards and to the unit of measurement realized at the corresponding national standard laboratory. This certificate may not be reproduced other than in full except with the prior written approval prior written approval of the calibration center, Play Solution Technology Co.,Ltd

# CERTIFICATE OF CALIBRATION

Certificate No. : PST-0126-24

W/O No. : WO-0051-24

Result of Calibration : Without Adjustment

Page no. 2 of 3

## 1. Repeatability

Weighing Range 1	g	Nominal Value	g	Standard Deviation	g
Max.capacity	220	50		0.000012	
		200		0.000048	

## 2. Linearity, Departure of Indication from nominal value

Weighing Range 1

Nominal Value	Standard Value	Indication	Error of Indication	Expanded Uncertainty	Factor k
g	g	g	g	g	
0.01	0.01000	0.01000	-0.000001	0.000082	2.87
0.1	0.10001	0.10001	0.000004	0.000082	2.87
0.5	0.50000	0.50001	0.000012	0.00008	2.87
1	1.00001	1.00002	0.000013	0.00008	2.87
5	5.00002	5.00003	0.000009	0.00008	2.52
10	9.99999	9.99999	-0.000001	0.00008	2.28
50	50.00001	49.99998	-0.000027	0.00016	2.00
100	100.00002	100.00002	0.000004	0.00030	2.00
150	150.00002	150.0001	0.000077	0.00045	2.00
200	200.00003	200.0001	0.000068	0.00060	2.00

# CERTIFICATE OF CALIBRATION

Certificate No. : PST-0126-24


W/O No. : WO-0051-24

## Result of Calibration

Page no. 3 of 3

### 3.Eccentricity

Test load at least 1/3 of the maximum capacity, typically placed between 1/2 and 1/3 of the distance from the centre of the load receptor to the edge.



Weighing Range 1

Test Load : 100 g

Position	Indication g
1	100.00004
2	100.00005
3	100.00002
4	100.00004
5	100.00003
Max.Deviation	0.00002

### Standard method

The calibration was performed by using calibration laboratory's in-house calibration method : CP-M-001 based on "UKAS LAB 14 : Calibration of weighing machine" : edition 6 | October 2019

### Reference standards instrument

Instrument	OIML Class	S/N	Certificate No.	Due Date
Standard Weight Set	E2	4000021952	22-128725	November 30, 2024
Standard Weight Set	-	-	-	-
Standard Weight Set	-	-	-	-
Standard Weight Set	-	-	-	-

### Measurement Uncertainty

The given measurement uncertainty is the standard of the measurement multiplied by an extension factor  $k$  which corresponds to a confidence level of about 95% for a normal distribution. The standard uncertainty was calculated according to UKAS M3003.

**Traceability :** The measurement is traceable to national standard, which realize the physical unit of measurement (SI)  
 - Through the reference calibration laboratory of Asia Medical and Agricultural Laboratory and Research Center Co.,Ltd


END OF REPORT



## High Volume Air Sampler Calibration Worksheet

Project Site :	Dcondo Ping Juristic Person Condominium	Barometric Pressure (mm Hg) :	730.5
Calibrate Location :	มมด้านหลังอาคาร C	Temperature ( °C ) :	31.7
Calibrate Date :	29-Oct-24	High Volume ID :	BKK_FS1056
CalibrationSheet No.:	C-291024-BKK_FS1056	High Volume Model :	TE-5009X
Calibrator ID:	BKK_FS0625	High Volume S/N :	5499
Calibrator Model :	TE-5028A	Calibrator Slope :	1.67329
Calibrator S/N :	2585	Calibrator Intercept :	-0.01925

Test No.	Delta H <sub>2</sub> O (inch)	Q <sub>std</sub> (m <sup>3</sup> /min)	I : Chart (CFM)	Linear Regression
1	3.2	1.0558	40	Slope : 34.6573 Intercept : 2.8069 Correlation Coefficient : 0.9979
2	4.2	1.2067	44	
3	5.4	1.3657	50	
4	6.4	1.4851	54	
5	7.8	1.6375	60	

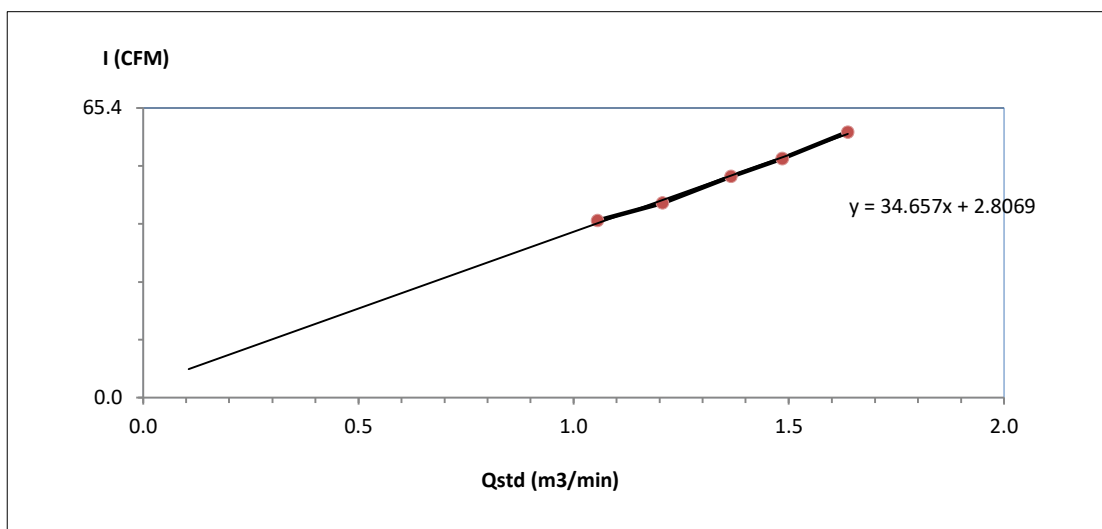

Calibrated by Jatsarawut

( Mr.Jatsarawut Pattama )  
Field Scientist(2)

Approved by : N. Noppong Juntarupan

(Mr. Noppong Juntarupan)  
Enviro Field Coordinator Scientist (3)

## Certificate of Calibration

### Customer

Name : ALS Laboratory Group Thailand Co., Ltd.  
Address : 104 Soi Phatthanakan 40, Phatthanakan Road, Suan Luang, Bangkok  
10250

Certificate No : 24-AFM-018 Rev.1

Request No : Req-2024-0043

### Unit Under Calibration Details

Measurement Item : Air Flow Meter  
Manufacturer : Bios  
Model : Defender 510-L  
Serial Number : 206895  
ID : BKK\_FS1346


Sensor Model : -

Sensor Serial Number : -

Location of Calibration : LAB 4 AIR VELOCITY METER

### Calibration Environment and Details

Temperature : 23 °C ± 3 °C  
Humidity : 55 %RH ± 20 %RH  
Barometric Pressure : 1013 hPa ± 10 hPa  
Received Date : 3 January 2024  
Calibration Date : 29 January 2024

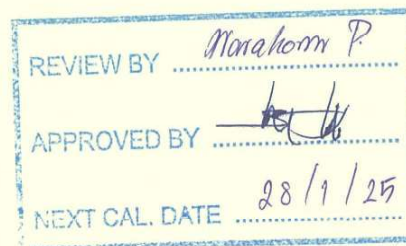

Calibration Procedure : In-house method CP-AFM-01 by Comparison technique with Standard Primary Flow Calibrator

Reference Standard	Model	Serial Number	Traceble	Due Calibration
Air Flow Meter	Gilibrator 3 Low flow	18501010006	Sensidyne	12 July 2024
Air Flow Meter	Gilibrator 3 Standard flow	19031011003	Sensidyne	12 July 2024
Temperature meter	GT 11	08000057	Qreborn	27 February 2024
Pressure meter	CPG2400	41000KDU/651882	TPA	9 November 2024

### Traceability :

This Certificate is traceable to SI Unit through Sensidyne A2LA Accreditation No. 3943.01

### Note :

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor  $k = 2$ , providing a level of confidence approximately 95 %.

This Certificate was issued to replace to Calibration Certificate No. 24-AFM-018

Calibration By : *ME*  
Mr. Noppadon Luangart  
Service Calibration Engineer

Approved By : *MSM*  
Mr. Pacit Mathavorn  
Calibration Engineer Supervisor

Issue Date : 1 February 2024

Certificate No : 24-AFM-018 Rev.1

Request No : Req-2024-0043

**Result of Calibration : Without Adjustment**

Temperature (°C)	Pressure (kPa)	STD (ml/min)	UUC (ml/min)	Error (ml/min)	Uncertainty (ml/min)
25.00	101.66	20	20.148	0.1	1.3
25.00	101.67	100	99.409	-0.6	2.8
24.90	101.63	199	197.46	-1.5	5.6
25.00	101.61	300	298.15	-1.8	8.4
24.90	101.60	399	400.13	1	11
24.90	101.59	480	478.02	-2.0	6.8

**Note**

STD : Standard UUC : Unit Under Calibration

- UUC Reference Condition : At atmospheric pressure and room temperature condition

- Flow Rate was corrected for non-standard operating condition by using equation :

$$Q_{\text{meas}} = Q_{\text{ref}} \times \frac{P_{\text{ref}}}{P_{\text{meas}}} \times \frac{T_{\text{meas}}}{T_{\text{ref}}}$$

where Q = Flow Rate P = Absolute Pressure T = Absolute Temperature

Meas = Measurement Condition ref = Standard Condition

\* Indicates non accredited

**End of Certificate**



NVLAP Lab Code 200661-0  
Calibration

## Calibration Certificate

**Certificate No.** 610563  
**Product** 200-510M Defender 510 Medium Flow  
**Serial No.** 151114  
**Cal. Date** 21-May-2024

**Sold To:**

All calibrations are performed in accordance with ISO 17025 at Mesa Laboratories, Inc., 12100 W. 6th Ave, Lakewood, CO 80228, an ISO 17025:2017 accredited laboratory through NVLAP. This report shall not be reproduced except in full without the written approval of the laboratory. Results only relate to the items calibrated. This report must not be used to claim product certification, approval, or endorsement by NVLAP, NIST, or any agency of the U.S. Government.

## As Received Calibration Data

**Technician** Derek Dellape  
**Lab. Pressure** 614.2 mmHg  
**Lab. Temperature** 24.3 °C

Instrument Reading	Lab Standard Reading	Deviation	Allowable Deviation	As Received
0 ccm	4504.81 ccm	-100.0%	1.00%	Out of Tolerance
0 ccm	1000.98 ccm	-100.0%	1.00%	Out of Tolerance
0 ccm	249.55 ccm	-100.0%	1.00%	Out of Tolerance

## Mesa Laboratories Standards Used

Description	Standard Serial Number	Calibration Date	Calibration Due Date
ML-800-24	117991	13-Nov-2023	13-Nov-2024

REVIEW BY	<i>W. Nakamura P.</i>
APPROVED BY	<i>[Signature]</i>
NEXT CAL. DATE	21/5/25

## As Shipped Calibration Data

<b>Certificate No</b>	610563	<b>Lab. Pressure</b>	617 mmHg
<b>Technician</b>	Derek Dellape	<b>Lab. Temperature</b>	24.6 °C

Instrument Reading	Lab Standard Reading	Deviation	Allowable Deviation	As Shipped
4482.47 ccm	4493.49 ccm	-0.25%	1.00%	In Tolerance
997.25 ccm	996.83 ccm	0.04%	1.00%	In Tolerance
248.51 ccm	248.67 ccm	-0.06%	1.00%	In Tolerance

## Mesa Laboratories Standards Used

Description	Standard Serial Number	Calibration Date	Calibration Due Date
ML-800-24	211063	04-Oct-2023	04-Oct-2024

### Calibration Notes

The expanded uncertainty of flow has a coverage factor of  $k = 2$  for a confidence interval of approximately 95%.

Flow testing is in accordance with our test number MP-00672 with an expanded uncertainty of 0.27% using high-purity nitrogen or filtered laboratory air.

Traceability to the International System of Units (SI) is verified by accreditation to ISO/IEC 17025 by NVLAP under NVLAP Code 200661-0.

### Technician Notes:

By:

Approved By:



Derek Dellape  
Production Assembler II



Troy Thacker  
Quality Engineer

Mesa Laboratories, Inc. certifies that the above instrument meets or exceeds published specifications, and that the calibration results in this certificate were obtained using equipment capable of producing results that are traceable through NIST to the International System of Units (SI). Calibration results are in compliance with ISO/IEC 17025:2017. Calibrations process has a Test Uncertainty Ratio (TUR) of 4:1 or greater. Any Pass/Fail determination is made without taking measurement uncertainty into account and is based on UUT performance against required tolerance only.

## Certificate of Calibration

### Customer

Name : ALS Laboratory Group Thailand Co., Ltd.  
Address : 104 Soi Phatthanakan 40, Phatthanakan Road, Suan Luang, Bangkok  
10250

Certificate No : 24-AFM-033

Request No : Req-2024-0241

### Unit Under Calibration Details

Measurement Item : Primary Flow Calibrator  
Manufacturer : Bios  
Model : Defender 510-L  
Serial Number : 130027  
ID : RYG\_FS0208  
Location of Calibration : LAB 4 AIR VELOCITY METER

Sensor Model : -

Sensor Serial Number : -

### Calibration Environment and Details

Temperature : 23 °C ± 3 °C  
Humidity : 55 %RH ± 20 %RH  
Barometric Pressure : 1013 hPa ± 10 hPa  
Received Date : 31 January 2024  
Calibration Date : 13 February 2024



Calibration Procedure : In-house method CP-AFM-01 by Comparison technique with Standard Primary Flow Calibrator

Reference Standard	Model	Serial Number	Traceble	Due Calibration
Air Flow Meter	Gilibrator 3 Low flow	18501010006	Sensidyne	12 July 2024
Air Flow Meter	Gilibrator 3 Standard flow	19031011003	Sensidyne	12 July 2024
Temperature meter	GT 11	08000057	Qreborn	27 February 2024
Pressure meter	CPG2400	41000KDU/651882	TPA	9 November 2024

### Traceability :

This Certificate is traceable to SI Unit through Sensidyne A2LA Accreditation No. 3943.01

### Note :

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor  $k = 2$ , providing a level of confidence approximately 95 %.

Calibration By : *[Signature]*  
Mr. Noppadon Luangart  
Service Calibration Engineer

Approved By : *[Signature]*  
Mr. Pacit Mathavorn  
Calibration Engineer Supervisor

Issue Date : 13 February 2024

Certificate No : 24-AFM-033

Request No : Req-2024-0241

**Result of Calibration : Without Adjustment**

Temperature (°C)	Pressure (kPa)	STD (cc/min)	UUC (cc/min)	Error (cc/min)	Uncertainty (cc/min)
24.50	101.26	20	19.965	0.0	1.3
24.20	101.25	101	100.50	-0.5	2.8
24.00	101.31	200	199.13	-0.9	5.6
23.90	101.42	301	303.56	2.6	8.4
24.10	101.41	401	404.57	4	11
24.10	101.49	480	483.81	3.8	7.0

**Note**

STD : Standard

UUC : Unit Under Calibration

- UUC Reference Condition : At atmospheric pressure and room temperature condition

- Flow Rate was corrected for non-standard operating condition by using equation :

$$Q_{\text{meas}} = Q_{\text{ref}} \times \frac{P_{\text{ref}}}{P_{\text{ref}}} \times \frac{T_{\text{meas}}}{T_{\text{ref}}}$$

where Q = Flow Rate

P = Absolute Pressure

T = Absolute Temperature

Meas = Measurement Condition

ref = Standard Condition

\* Indicates non accredited

**End of Certificate**

## Certificate of Calibration

### Customer

Name : ALS Laboratory Group Thailand Co., Ltd.  
Address : 104 Soi Phatthanakan 40, Phatthanakan Road, Suan Luang, Bangkok  
10250

Certificate No : 24-AFM-032

Request No : Req-2024-0240

### Unit Under Calibration Details

Measurement Item : Primary Flow Calibrator  
Manufacturer : Bios  
Model : Defender 510-M  
Serial Number : 129958  
ID : RYG\_FS0209  
Sensor Model : -  
Sensor Serial Number : -  
Location of Calibration : LAB 4 AIR VELOCITY METER

### Calibration Environment and Details

Temperature : 23 °C ± 3 °C  
Humidity : 55 %RH ± 20 %RH  
Barometric Pressure : 1013 hPa ± 10 hPa  
Received Date : 31 January 2024  
Calibration Date : 13 February 2024



Calibration Procedure : In-house method CP-AFM-01 by Comparison technique with Standard Primary Flow Calibrator

Reference Standard	Model	Serial Number	Traceble	Due Calibration
Air Flow Meter	Gilibrator 3 Low flow	18501010006	Sensidyne	12 July 2024
Air Flow Meter	Gilibrator 3 Standard flow	19031011003	Sensidyne	12 July 2024
Temperature meter	GT 11	08000057	Qreborn	27 February 2024
Pressure meter	CPG2400	41000KDU/651882	TPA	9 November 2024

### Traceability :

This Certificate is traceable to SI Unit through Sensidyne A2LA Accreditation No. 3943.01

### Note :

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor  $k = 2$ , providing a level of confidence approximately 95 %.

Calibration By : *me*  
Mr. Noppadon Luangart  
Service Calibration Engineer

Approved By : *Mr. Pacit Mathavorn*  
Mr. Pacit Mathavorn  
Calibration Engineer Supervisor

Issue Date : 13 February 2024

Certificate No : 24-AFM-032

Request No : Req-2024-0240

**Result of Calibration : Without Adjustment**

Temperature (°C)	Pressure (kPa)	STD (cc/min)	UUC (cc/min)	Error (cc/min)	Uncertainty (cc/min)
23.80	101.89	95	100.13	5.1	2.8
23.90	101.71	501	513.93	12.9	7.2
24.18	101.62	1006	1019.3	13	14
24.00	101.81	1997	2023.0	26	29
24.10	101.87	2999	3035.5	37	45
24.60	102.00	3944	3991.8	48	59
24.60	102.08	4739	4790.5	52	72

**Note**

STD : Standard

UUC : Unit Under Calibration

- UUC Reference Condition : At atmospheric pressure and room temperature condition

- Flow Rate was corrected for non-standard operating condition by using equation :

$$Q_{meas} = Q_{ref} \times \frac{P_{ref}}{P_{meas}} \times \frac{T_{meas}}{T_{ref}}$$

where Q = Flow Rate

P = Absolute Pressure

T = Absolute Temperature

Meas = Measurement Condition

ref = Standard Condition

\* Indicates non accredited

**End of Certificate**

## Certificate of Calibration

### Customer

Name : ALS Laboratory Group Thailand Co., Ltd.  
Address : 104 Soi Phatthanakan 40, Phatthanakan Road, Suan Luang,  
Bangkok 10250

Certificate No : 24-AFM-174

Request No : Req-2024-1861

### Unit Under Calibration Details

Measurement Item : Air Flow Meter  
Manufacturer : MesaLabs  
Model : 510-M  
Serial Number : 208345  
ID : BKK\_FS1347  
Location of Calibration : LAB 4 AIR VELOCITY METER

Accuracy : 1% of Reading  
Sensor Model : -  
Sensor Serial Number : -  
Instrument Status : Used

### Calibration Environment and Details

Temperature : 23 °C ± 3 °C  
Humidity : 55 %RH ± 20 %RH  
Barometric Pressure : 1013 hPa ± 10 hPa  
Received Date : 22 August 2024  
Calibration Date : 28 August 2024

REVIEW BY	<i>Manakorn P.</i>
APPROVED BY	<i>[Signature]</i>
NEXT CAL. DATE	28/8/25

Calibration Procedure : In-house method CP-AFM-01 by Comparison technique with Standard Primary Flow Calibrator

Reference Standard	Model	Serial Number	Traceble	Due Calibration
Air Flow Meter	Gilibrator 3 Low flow	18501010006	Sensidyne	6 August 2025
Air Flow Meter	Gilibrator 3 Standard flow	19031011003	Sensidyne	2 August 2025
Temperature meter	GT 11	08000057	Qreborn	1 March 2025
Pressure meter	CPG2400	41000KDU/651882	TPA	9 November 2024

### Traceability :

This Certificate is traceable to SI Unit through Sensidyne A2LA Accreditation No. 3943.01

### Note :

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor  $k = 2$ , providing a level of confidence approximately 95 %.

Calibration By : *me*  
Mr. Noppadon Luangart  
Service Calibration Engineer

Approved By : *ปวิญ*  
Mr. Pacit Mathavorn  
Calibration Engineer Supervisor

Issue Date : 28 August 2024

Certificate No : 24-AFM-174

Request No : Req-2024-1861

**Result of Calibration : Without Adjustment**

Temperature (°C)	Pressure (kPa)	STD (cc/min)	UUC (cc/min)	Error (cc/min)	Uncertainty (cc/min)	MPE (cc/min)	Result
22.30	100.57	100	99.526	-0.5	2.8	1	N/A
22.40	100.61	499	500.48	1.5	7.8	5	N/A
22.50	100.56	1004	1004.8	1	15	10	N/A
22.60	100.54	2008	2003.3	-5	29	20	N/A
22.80	100.62	3034	3032.1	-2	45	30	N/A
23.20	100.71	4032	4022.4	-10	60	40	N/A
23.40	100.73	5060	5056.4	-4	79	51	N/A

**Note**

STD : Standard UUC : Unit Under Calibration

- UUC Reference Condition : At atmospheric pressure and room temperature condition

- Flow Rate was corrected for non-standard operating condition by using equation :

$$Q_{meas} = Q_{ref} \times \frac{P_{ref}}{P_{meas}} \times \frac{T_{meas}}{T_{ref}}$$

where Q = Flow Rate

P = Absolute Pressure

T = Absolute Temperature

Meas = Measurement Condition

ref = Standard Condition

\* Indicates non accredited

MPE = Maximum Permissible Error (Specified in Manufacturer's Specifications)

N/A = Not Available, Customer does not require a statement of conformity.

Certificate No : 24-AFM-174

Request No : Req-2024-1861

### Decision Rule for Statements of Conformity


The standard decision rule employed for the statements of conformity to each calibration result will be applied using ILAC-G8:09/2019; Guidelines on the Reporting of Compliance with Specification as following Fig. and statements

Pass = The measurement result plus the expanded uncertainty with a 95% coverage probability were within the limit.

Pass<sup>1</sup> = The measurement result was within the limit. However, a portion of the expanded uncertainty of measurement at 95% exceeds the limit.

Fail<sup>1</sup> = The measurement result was out of the limit. However, a portion of the expanded uncertainty of measurement at 95% is within the limit.

Fail = The measurement result plus the expanded uncertainty with a 95% coverage probability were outside the limit.

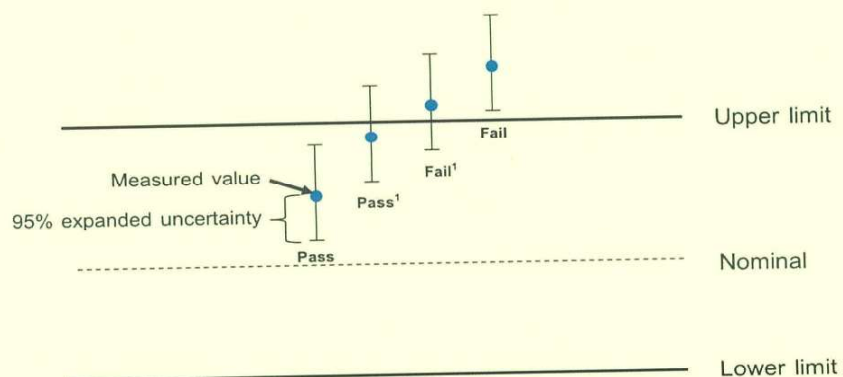

End of Certificate

## Certificate of Calibration

### Customer

Name : ALS Laboratory Group Thailand Co., Ltd.  
Address : 104 Soi Phatthanakan 40, Phatthanakan Road, Suan Luang,  
Bangkok 10250

Certificate No : 24-AFM-177

Request No : Req-2024-1862

### Unit Under Calibration Details

Measurement Item : Air Flow Meter  
Manufacturer : Bios Accuracy : 1% of Reading  
Model : Defender 510-L Sensor Model : -  
Serial Number : 130026 Sensor Serial Number : -  
ID : BKK\_FS0619 Instrument Status : Used  
Location of Calibration : LAB 4 AIR VELOCITY METER

### Calibration Environment and Details

Temperature : 23 °C ± 3 °C  
Humidity : 55 %RH ± 20 %RH  
Barometric Pressure : 1013 hPa ± 10 hPa  
Received Date : 22 August 2024  
Calibration Date : 9 September 2024  
Calibration Procedure : In-house method CP-AFM-01 by Comparison technique with Standard Primary Flow Calibrator



Reference Standard	Model	Serial Number	Traceble	Due Calibration
Air Flow Meter	Gilibrator 3 Low flow	18501010006	Sensidyne	6 August 2025
Air Flow Meter	Gilibrator 3 Standard flow	19031011003	Sensidyne	2 August 2025
Temperature meter	GT 11	08000057	Qreborn	1 March 2025
Pressure meter	CPG2400	41000KDU/651882	TPA	9 November 2024

### Traceability :

This Certificate is traceable to SI Unit through Sensidyne A2LA Accreditation No. 3943.01

### Note :

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor  $k = 2$ , providing a level of confidence approximately 95 %.

Calibration By : *[Signature]*  
Mr. Noppadon Luangart  
Service Calibration Engineer

Approved By : *[Signature]*  
Mr. Pacit Mathavorn  
Calibration Engineer Supervisor

Issue Date : 9 September 2024

Certificate No : 24-AFM-177

Request No : Req-2024-1862

**Result of Calibration : Without Adjustment**

Temperature (°C)	Pressure (kPa)	STD (cc/min)	UUC (cc/min)	Error (cc/min)	Uncertainty (cc/min)	MPE (cc/min)	Result
24.70	100.92	20	20.192	0.2	1.3	0.2	N/A
24.70	100.90	100	99.923	-0.1	2.8	1.0	N/A
24.70	100.94	201	200.7	-0.3	5.6	2.0	N/A
24.70	100.97	298	300.1	2.1	8.4	3.0	N/A
24.70	100.99	403	399.1	-4	11	4.0	N/A
24.80	101.05	482	477.6	-4.4	6.9	4.8	N/A

**Note**

STD : Standard UUC : Unit Under Calibration

- UUC Reference Condition : At atmospheric pressure and room temperature condition

- Flow Rate was corrected for non-standard operating condition by using equation :

$$Q_{meas} = Q_{ref} \times \frac{P_{ref}}{P_{meas}} \times \frac{T_{meas}}{T_{ref}}$$

where Q = Flow Rate

P = Absolute Pressure

T = Absolute Temperature

Meas = Measurement Condition

ref = Standard Condition

\* Indicates non accredited

MPE = Maximum Permissible Error (Specified in Manufacturer's Specifications)

N/A = Not Available, Customer does not require a statement of conformity.

Certificate No : 24-AFM-177

Request No : Req-2024-1862

### Decision Rule for Statements of Conformity


The standard decision rule employed for the statements of conformity to each calibration result will be applied using ILAC-G8:09/2019; Guidelines on the Reporting of Compliance with Specification as following Fig. and statements

Pass = The measurement result plus the expanded uncertainty with a 95% coverage probability were within the limit.

Pass<sup>1</sup> = The measurement result was within the limit. However, a portion of the expanded uncertainty of measurement at 95% exceeds the limit.

Fail<sup>1</sup> = The measurement result was out of the limit. However, a portion of the expanded uncertainty of measurement at 95% is within the limit.

Fail = The measurement result plus the expanded uncertainty with a 95% coverage probability were outside the limit.

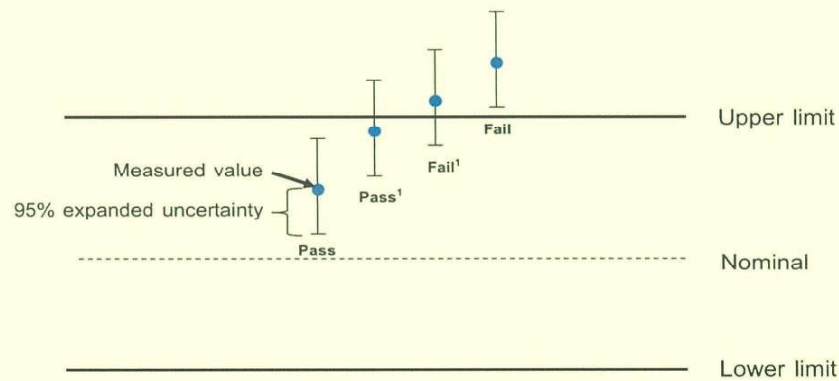

End of Certificate


TEST REPORT

REVIEW BY Vichuta N.  
APPROVED BY Tanyatorn M.  
NEXT CAL. DATE 11/6/25


CUSTOMER NAME	: ALS Laboratory Group (Thailand) Co., Ltd. [บริษัท เอแอลเอส แล็บอราทอรี กรุ๊ป (ประเทศไทย) จำกัด]						
EQUIPMENT NAME	: THC Analyzer						
MANUFACTURER	: HORIBA	MODEL	: APHA-370	SERIAL NO	: WKJ0NS9M		
STANDARD GAS CONCENTRATION (PPM)	: 506.1 PPM			CYLINDER NO	: CC734373		
CYLINDER PRESSURE (psig)	: 1,000 PSI			CERTIFIED DATE	: 12/05/2020		
CERTIFIED BY	: AIRGAS			EXPIRED DATE	: 12/05/2028		

TEST RESULTS

POINT NO	TEST RESULTS						
	IDEAL	ACTUAL CH4	ERROR CH4	%ERROR CH4	ACTUAL THC	ERROR THC	%ERROR THC
ZERO	0.000	0.00	0.000	-	0.00	0.000	-
1	10.000	10.30	0.300	3.00	10.29	0.290	2.90
2	20.000	20.20	0.200	1.00	20.09	0.090	0.45
3	30.000	30.01	0.010	0.03	30.10	0.100	0.33
4	40.000	39.90	-0.100	-0.25	39.99	-0.010	-0.02
AVERAGE (%)				0.95	0.91		

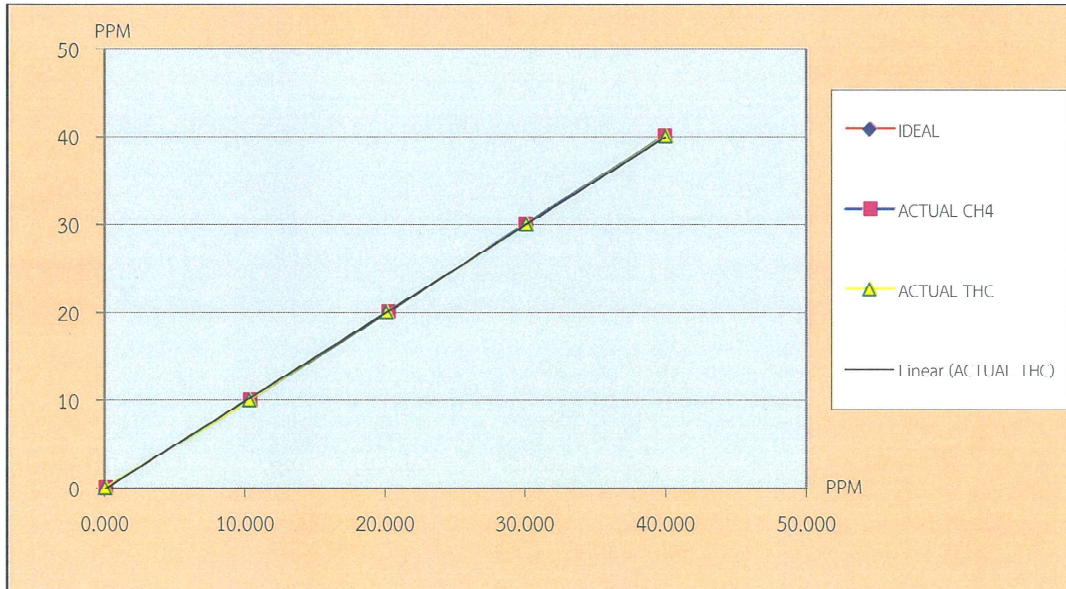

CALIBRATED BY : วชิราภรณ์ อรุณวงศ์ DATE : 11/12/66  
CHECKED BY : สจ. วิภาณี DATE : 11/12/66



ต้องการข้อมูลทางด้านเทคนิคเพิ่มเติม : เจ้าหน้าที่ฝ่ายบริการหลังการขาย , โทร 02-868-0812 # 15,16 , E-Mail : Engineer@jiranatee.com  
เลขที่ 63/14-15,67/35-36 ถนนเพชรเกษม 7,7/1 แขวงวัดท่าพระ เขตบางกอกใหญ่ กรุงเทพฯ 10600 โทร 02-8680812-13 โทรสาร 02-868-1889

# MULTI POINT CALIBRATION REPORT

CUSTOMER NAME : ALS Laboratory Group (Thailand) Co.Ltd.

EQUIPMENT NAME : CO Analyzer

MANUFACTURER : Teledyne - API

MODEL : T300

SERIAL NO : 5947

STANDARD GAS CONCENTRATION (PPM) : 808.9

CERTIFIED DATE : CC739972

CYLINDER PRESSURE (psig) : 900

CERTIFIED DATE : Nov ,05 ,2020

CERTIFIED BY : AIRGAS SPECIALTY GASES

EXPIRED DATE : Nov ,05, 2028


## CALIBRATION RESULTS

POINT NO	CALIBRATION RESULTS			
	IDEAL (PPM)	ACTUAL CO (PPM)	ERROR CO (PPM)	% ERROR CO
ZERO	0.00	0.01	0.01	-
1	50.00	49.36	-0.64	-1.28
2	90.00	89.54	-0.46	-0.51
3	199.20	202.08	2.88	1.45
4	400.30	402.41	2.11	0.53
5	808.90	808.47	-0.43	-0.05
AVERAGE (%)				0.76

REVIEW BY Vichufa N.

APPROVED BY Tanvatoon M.

NEXT CAL. DATE 5 Aug 95

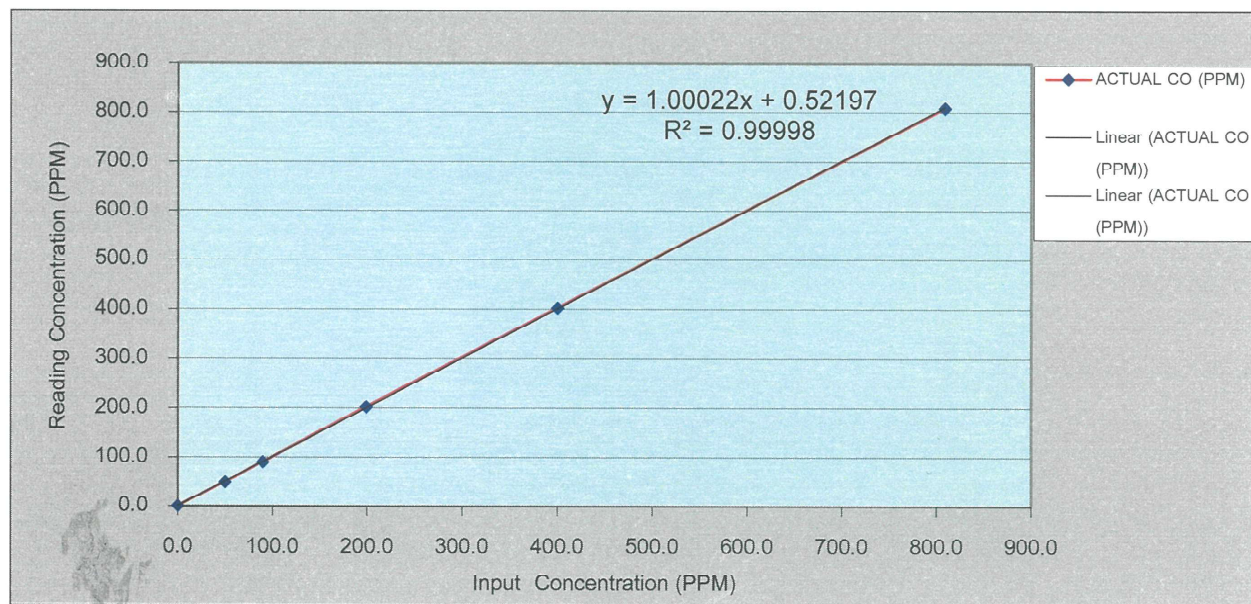

CALIBRATED BY : คุณธนาคม มหาอาจ

DATE : 5 สิงหาคม 2567

ต้องการข้อมูลทางด้านเทคนิคเพิ่มเติม : คุณธนาคม มหาอาจ โทรศัพท์ : 02-515-8987