

ภาคผนวก ค

ใบรายงานผลวิเคราะห์คุณภาพน้ำ

ภาคผนวก ค-1
ใบรายงานผลวิเคราะห์คุณภาพน้ำทิ้ง

Analysis/Test Report

Customer Name : The Iconsiam Superlux Residence Condominium Juristic Person

Address : 289 Charoen Nakhon Road, Khlong San, Bangkok 10600, Thailand

Sampling Site : Residences at Mandarin Oriental Bangkok

Sample Type : Waste Water

Sampling by : Test Tech Co., Ltd.

Sampling Method : Grab

Sampling Date : 04/07/2024

Sampling Time : 10:40 AM

Received Date : 04/07/2024

Analytical Date : 04 - 11/07/2024

Report Date : 12/07/2024

Report No. : R16747/67

Parameters	Unit	Method	TW15345 /67	Standard ^a (Type B)
			Waste Water Effluent Tank	
pH	-	SM 2023 (4500-H ⁺ B)	7.6	5.0 - 9.0
BOD	mg/L	SM 2023 (5210 B, 4500-O G)	4.8	≤ 30
* Total Suspended Solids	mg/L	SM 2023 (2540 D)	1	≤ 40
Total Dissolved Solids	mg/L	Based on SM 2023 (2540 C)	268	500 ^{xx}
Oil & Grease	mg/L	SM 2023 (5520 D)	< 3.0	≤ 20
Total Kjeldahl Nitrogen	mg/L as N	SM 2023 (4500 N _{org} B)	2.8	≤ 35
* Sulfide	mg/L as H ₂ S	Iodometric	< 0.30	≤ 1.0
* Settleable Solids	mL/L	Volumetric Test	< 0.5	≤ 0.5
Sample Condition		Observation	Light Yellow, Clear	

Remark : 1. SM 2023 : Standard Methods for the Examination of Water and Wastewater, APHA, AWWA & WEF, 24th ed., 2023

2. Test marked " * " on this report are not included in scope of Accreditation

3. a : Notification of Ministry of Natural Resources and Environment : Building Effluents Standards Published in the Royal Government Gazette, Vol.122 Part 125 D, dated December 29, B.E.2548 (2005)

^{xx} These values are in addition to the TDS of the water used.

S. Busaya

Miss BUSAYA SRISAWANG

Analyst

12/07/2024



Miss ORASA YUBUA

Technical Manager

12/07/2024

Reported results refer to the sample as received only.

Test report shall not be reproduced except in full, without written approved of the laboratory.

The laboratory has been accepted as an accredited laboratory complying with the ISO/IEC 17025

TESTING
NO.0001

Analysis/Test Report

Customer Name : The Iconsiam Superlux Residence Condominium Juristic Person

Address : 289 Charoen Nakhon Road, Khlong San, Bangkok 10600, Thailand

Sampling Site : Residences at Mandarin Oriental Bangkok

Sample Type : Waste Water

Sampling by : Test Tech Co., Ltd.

Sampling Method : Grab

Sampling Date : 06/08/2024

Sampling Time : 11:00 AM

Received Date : 07/08/2024

Analytical Date : 07 - 13/08/2024

Report Date : 15/08/2024

Report No. : R19550/67

Parameters	Unit	Method	TW18025 /67	Standard ^a (Type B)
			Waste Water	
pH	-	SM 2023 (4500-H ⁺ B)	7.7	5.0 - 9.0
BOD	mg/L	SM 2023 (5210 B, 4500-O G)	3.1	≤ 30
* Total Suspended Solids	mg/L	SM 2023 (2540 D)	2	≤ 40
Total Dissolved Solids	mg/L	Based on SM 2023 (2540 C)	284	500 ^{xx}
Oil & Grease	mg/L	SM 2023 (5520 D)	< 3.0	≤ 20
Total Kjeldahl Nitrogen	mg/L as N	SM 2023 (4500 N _{org} B)	< 2.0	≤ 35
* Sulfide	mg/L as H ₂ S	Iodometric	< 0.30	≤ 1.0
* Settleable Solids	mL/L	Volumetric Test	< 0.5	≤ 0.5
Sample Condition		Observation	Colorless, a little bit Particles	

Remark : 1. SM 2023 : Standard Methods for the Examination of Water and Wastewater, APHA, AWWA & WEF, 24th ed., 2023

2. Test marked " * " on this report are not included in scope of Accreditation

3. a : Notification of Ministry of Natural Resources and Environment : Building Effluents Standards Published in the Royal Government Gazette, Vol.122 Part 125 D, dated December 29, B.E.2548 (2005)

^{xx} These values are in addition to the TDS of the water used.

S. Busaya

Miss BUSAYA SRISAWANG

Analyst

15/08/2024



Miss BUSAYA SRISAWANG

Technical Manager

15/08/2024

Reported results refer to the sample as received only.

Test report shall not be reproduced except in full, without written approved of the laboratory.

The laboratory has been accepted as an accredited laboratory complying with the ISO/IEC 17025

TESTING
NO.0001

Analysis/Test Report

Customer Name : The Iconsiam Superlux Residence Condominium Juristic Person

Address : 289 Charoen Nakhon Road, Khlong San, Bangkok 10600, Thailand

Sampling Site : Residences at Mandarin Oriental Bangkok

Sample Type : Waste Water

Sampling by : Test Tech Co., Ltd.

Sampling Method : Grab

Sampling Date : 09/09/2024

Sampling Time : 11:00 AM

Received Date : 10/09/2024

Analytical Date : 10 - 16/09/2024

Report Date : 17/09/2024

Report No. : R22606/67

Parameters	Unit	Method	TW20788 /67	Standard ^a (อาคารประเภท ข)
			Waste Water Effluent Tank	
pH	-	SM 2023 (4500-H ⁺ B)	7.4	5.5 - 9.0
BOD	mg/L	SM 2023 (5210 B, 4500-O G)	4.4	≤ 30
* Total Suspended Solids	mg/L	SM 2023 (2540 D)	2	≤ 40
Total Dissolved Solids	mg/L	SM 2023 (2540 C)	392	≤ 1,000
Oil & Grease	mg/L	SM 2023 (5520 D)	< 3.0	≤ 20
Total Kjeldahl Nitrogen	mg/L as N	SM 2023 (4500 N _{org} B)	< 2.0	≤ 35
* Sulfide	mg/L as H ₂ S	Iodometric	< 0.30	≤ 1.0
* Settleable Solids	mL/L	Volumetric Test	< 0.5	-
Sample Condition		Observation	Light Yellow, Clear	

Remark : 1. SM 2023 : Standard Methods for the Examination of Water and Wastewater, APHA, AWWA & WEF, 24th ed., 2023

2. Test marked " * " on this report are not included in scope of Accreditation

3. a : อ้างอิงตามประกาศกระทรวงทรัพยากรธรรมชาติและสิ่งแวดล้อม เรื่อง กำหนดมาตรฐานควบคุมการระบายน้ำทิ้งจากอาคาร
บางประเภทและบางขนาด พ.ศ. 2567

S. Busaya

Miss BUSAYA SRISAWANG

Analyst

17/09/2024



Miss ORISA YUBUA

TEST TECH CO., LTD.

Technical Manager

17/09/2024

Reported results refer to the sample as received only.

Test report shall not be reproduced except in full, without written approved of the laboratory.

The laboratory has been accepted as an accredited laboratory complying with the ISO/IEC 17025

Analysis/Test Report

Customer Name : The Iconsiam Superlux Residence Condominium Juristic Person

Address : 289 Charoen Nakhon Road, Khlong San, Bangkok 10600, Thailand

Sampling Site : Residences at Mandarin Oriental Bangkok

Sample Type : Waste Water

Sampling by : Test Tech Co., Ltd.

Sampling Method : Grab

Sampling Date : 07/10/2024

Sampling Time : 10:55 AM

Received Date : 07/10/2024

Analytical Date : 07 - 15/10/2024

Report Date : 17/10/2024

Report No. : R24895/67

Parameters	Unit	Method	TW22935 /67	^a Standard
			Waste Water	(อาคารประเภท ข)
pH	-	SM 2023 (4500-H ⁺ B)	7.6	5.5 - 9.0
BOD	mg/L	SM 2023 (5210 B, 4500-O G)	3.8	≤ 30
* Total Suspended Solids	mg/L	SM 2023 (2540 D)	1	≤ 40
Total Dissolved Solids	mg/L	SM 2023 (2540 C)	460	≤ 1,000
Oil & Grease	mg/L	SM 2023 (5520 D)	< 3.0	≤ 20
Total Kjeldahl Nitrogen	mg/L as N	SM 2023 (4500 N _{org} B)	< 2.0	≤ 35
* Sulfide	mg/L as H ₂ S	Iodometric	< 0.30	≤ 1.0
* Settleable Solids	mL/L	Volumetric Test	< 0.5	-
Sample Condition		Observation	Light Yellow, Clear	

Remark : 1. SM 2023 : Standard Methods for the Examination of Water and Wastewater, APHA, AWWA & WEF, 24th ed., 2023

2. Test marked " * " on this report are not included in scope of Accreditation

3. a : อ้างอิงตามประกาศกระทรวงทรัพยากรธรรมชาติและสิ่งแวดล้อม เรื่อง กำหนดมาตรฐานควบคุมการระบายน้ำทิ้งจากอาคาร
บางประเภทและบางขนาด พ.ศ. 2567

S. Busaya

Miss BUSAYA SRISAWANG

Analyst

17/10/2024

บริษัท เทสต์ เทค จำกัด

Y. CRASA

Miss CRASA YUBUA

TEST TECH CO., LTD.

Technical Manager

17/10/2024

Reported results refer to the sample as received only.

Test report shall not be reproduced except in full, without written approved of the laboratory.

The laboratory has been accepted as an accredited laboratory complying with the ISO/IEC 17025



Analysis/Test Report

Customer Name : The Iconsiam Superlux Residence Condominium Juristic Person

Address : 289 Charoen Nakhon Road, Khlong San, Bangkok 10600, Thailand

Sampling Site : Residences at Mandarin Oriental Bangkok

Sample Type : Waste Water

Sampling by : Test Tech Co., Ltd.

Sampling Method : Grab

Sampling Date : 12/11/2024

Sampling Time : 11:50 AM

Received Date : 13/11/2024

Analytical Date : 13 - 18/11/2024

Report Date : 19/11/2024

Report No. : R27668/67

Parameters	Unit	Method	TW25582 /67	Standard ^a (อาคารประเภท ข)
			Waste Water	
pH	-	SM 2023 (4500-H ⁺ B)	7.5	5.5 - 9.0
BOD	mg/L	SM 2023 (5210 B, 4500-O G)	6.0	≤ 30
Total Suspended Solids	mg/L	SM 2023 (2540 D)	8	≤ 40
Total Dissolved Solids	mg/L	SM 2023 (2540 C)	288	≤ 1,000
Oil & Grease	mg/L	SM 2023 (5520 D)	< 3.0	≤ 20
Total Kjeldahl Nitrogen	mg/L as N	SM 2023 (4500 N _{org} B)	5.6	≤ 35
Sulfide	mg/L as H ₂ S	Iodometric	< 0.30	≤ 1.0
Settleable Solids	mL/L	Volumetric Test	< 0.5	-
Sample Condition		Observation	Light Yellow, a little bit Particles	

Remark : 1. SM 2023 : Standard Methods for the Examination of Water and Wastewater, APHA, AWWA & WEF, 24th ed., 2023

2. Test marked " * " on this report are not included in scope of Accreditation

3. a : อ้างอิงตามประกาศกระทรวงทรัพยากรธรรมชาติและสิ่งแวดล้อม เรื่อง กำหนดมาตรฐานควบคุมการระบายน้ำทิ้งจากอาคาร
บางประเภทและบางขนาด พ.ศ. 2567

S. Busaya

Miss BUSAYA SRISAWANG

Analyst

19/11/2024



19/11/2024

Reported results refer to the sample as received only.

Test report shall not be reproduced except in full, without written approved of the laboratory.

The laboratory has been accepted as an accredited laboratory complying with the ISO/IEC 17025

Analysis/Test Report

Customer Name : The Iconsiam Superlux Residence Condominium Juristic Person

Address : 289 Charoen Nakhon Road, Khlong San, Bangkok 10600, Thailand

Sampling Site : Residences at Mandarin Oriental Bangkok

Sample Type : Waste Water

Sampling by : Test Tech Co., Ltd.

Sampling Method : Grab

Sampling Date : 10/12/2024

Sampling Time : 10:40 AM

Received Date : 11/12/2024

Analytical Date : 11 - 16/12/2024

Report Date : 17/12/2024

Report No. : R29926/67

Parameters	Unit	Method	TW27766 /67	Standard ^a (อาคารประเภท ข)
			Waste Water	
pH	-	SM 2023 (4500-H ⁺ B)	7.4	5.5 - 9.0
BOD	mg/L	SM 2023 (5210 B, 4500-O G)	10	≤ 30
Total Suspended Solids	mg/L	SM 2023 (2540 D)	34	≤ 40
Total Dissolved Solids	mg/L	SM 2023 (2540 C)	234	≤ 1,000
Oil & Grease	mg/L	SM 2023 (5520 D)	< 3.0	≤ 20
Total Kjeldahl Nitrogen	mg/L as N	SM 2023 (4500 N _{org} B)	4.9	≤ 35
* Sulfide	mg/L as H ₂ S	Iodometric	< 0.30	≤ 1.0
* Settleable Solids	mL/L	Volumetric Test	< 0.5	-
Sample Condition		Observation	Light Yellow, Colloid	

Remark : 1. SM 2023 : Standard Methods for the Examination of Water and Wastewater, APHA, AWWA & WEF, 24th ed., 2023

2. Test marked " * " on this report are not included in scope of Accreditation

3. a : อ้างอิงตามประกาศกระทรวงทรัพยากรธรรมชาติและสิ่งแวดล้อม เรื่อง กำหนดมาตรฐานควบคุมการระบายน้ำทิ้งจากอาคาร
บางประเภทและบางขนาด พ.ศ. 2567

S. Ployrung

Miss PLOYRUNG SUTHAMMA

Analyst

17/12/2024


Miss ORISA YUBUA
TEST TECH CO., LTD.

Technical Manager

17/12/2024

Reported results refer to the sample as received only.

Test report shall not be reproduced except in full, without written approved of the laboratory.

The laboratory has been accepted as an accredited laboratory complying with the ISO/IEC 17025

ภาคผนวก ค-2
ใบรายงานผลวิเคราะห์คุณภาพน้ำใช้



Analysis/Test Report

Customer Name : The Iconsiam Superlux Residence Condominium Juristic Person

Address : 289 Charoen Nakhon Road, Khlong San, Bangkok 10600, Thailand

Sampling Site : Residences at Mandarin Oriental Bangkok

Sample Type : Water Supply

Sampling by : Test Tech Co., Ltd.

Sampling Method : Grab

Sampling Date : 04/07/2024

Sampling Time : 10:40 AM

Received Date : 04/07/2024

Analytical Date : 04 - 08/07/2024

Report Date : 11/07/2024

Report No. : R16513/67

Parameters	Unit	Method	TW15344 /67
			Water Supply
Total Dissolved Solids	mg/L	Based on SM 2023 (2540 C)	158
Sample Condition			Clear

Remark : 1. SM 2023 : Standard Methods for the Examination of Water and Wastewater, APHA, AWWA & WEF, 24th ed., 2023

S. Ployrung

Miss PLOYRUNG SUTHAMMA

Analyst

11/07/2024



Miss ORASA YUBUA

Technical Manager

11/07/2024

Reported results refer to the sample as received only.

Test report shall not be reproduced except in full, without written approved of the laboratory.

The laboratory has been accepted as an accredited laboratory complying with the ISO/IEC 17025



Analysis/Test Report

Customer Name : The Iconsiam Superlux Residence Condominium Juristic Person

Address : 289 Charoen Nakhon Road, Khlong San, Bangkok 10600, Thailand

Sampling Site : Residences at Mandarin Oriental Bangkok

Sample Type : Water Supply

Sampling by : Test Tech Co., Ltd.

Sampling Method : Grab

Sampling Date : 06/08/2024

Sampling Time : 11:00 AM

Received Date : 07/08/2024

Analytical Date : 07 - 10/08/2024

Report Date : 13/08/2024

Report No. : R19363/67

Parameters	Unit	Method	TW18024 /67
			Water Supply
Total Dissolved Solids	mg/L	Based on SM 2023 (2540 C)	164
Sample Condition			Clear

Remark : 1. SM 2023 : Standard Methods for the Examination of Water and Wastewater, APHA, AWWA & WEF, 24th ed., 2023

S. Ployrung

Miss PLOYRUNG SUTHAMMA

Analyst

13/08/2024



Technical Manager

13/08/2024

Reported results refer to the sample as received only.

Test report shall not be reproduced except in full, without written approved of the laboratory.

The laboratory has been accepted as an accredited laboratory complying with the ISO/IEC 17025

ภาคผนวก ค-3

ใบรายงานผลวิเคราะห์คุณภาพน้ำสระว่ายนํ้า

Analysis/Test Report

Customer Name : The Iconsiam Superlux Residence Condominium Juristic Person

Address : 289 Charoen Nakhon Road, Khlong San, Bangkok 10600, Thailand

Sampling Site : Residences at Mandarin Oriental Bangkok

Sample Type : Swimming Water

Sampling by : Test Tech Co., Ltd.

Sampling Method : Grab

Sampling Date : 04/07/2024

Sampling Time : 09:50 AM

Received Date : 04/07/2024

Analytical Date : 04 - 09/07/2024

Report Date : 11/07/2024

Report No. : R16623/67

Parameters	Unit	Method	TW15346 /67	Standard ^a	Standard ^b
			Swimming Pool-Main		
pH (25°C)	-	Based on SM 2023 (4500-H ⁺ B)	7.3	7.2-7.4	7.2-7.4
Dissolved Solids	mg/L as NaCl	Electrical Conductivity	3684	xx	xx
Total Alkalinity	mg/L as CaCO ₃	Titration	25	-	-
Calcium Hardness	mg/L as CaCO ₃	EDTA Titrimetric	106	75-150	75-150
Chloride	mg/L as Cl ⁻	SM 2023 (4500-Cl ⁻ B)	1859	0-600	0-600
Sulfate	mg/L as SO ₄ ²⁻	Based on SM 2023 (4500-SO ₄ ²⁻ E)	9.46	0-200	0-200
Free Chlorine	mg/L as Cl ₂	DPD Colorimetric	1.21	0.5	1.1-2.2
Combine Chlorine	mg/L as Cl ₂	DPD Colorimetric	0.37	x	x
Cyanuric acid	mg/L	Colorimetric	4	50-100	50-100
Bromine	mg/L	DPD Colorimetric	3.16	4.0-6.0	4.0-6.0
Sample Condition		Observation	Clear		

Remark : 1. SM 2023 : Standard Methods for the Examination of Water and Wastewater, APHA, AWWA & WEF, 24th ed., 2023

2. a : Standard from Customer

x : Less than half the free chlorine or 1.0 whichever is less

xx : < 1000 above source water

3. b : Standard from Customer

x : Less than half the free chlorine or 1.0 whichever is less

xx : < 1000 above source water

R. Prangtip

Miss PRANGTIP RAKSASUK

Analyst

11/07/2024



Miss ORASA YUBUA

Technical Manager

11/07/2024

Reported results refer to the sample as received only.

Test report shall not be reproduced except in full, without written approved of the laboratory.

The laboratory has been accepted as an accredited laboratory complying with the ISO/IEC 17025

TESTING
NO.0001

Analysis/Test Report

Customer Name : The Iconsiam Superlux Residence Condominium Juristic Person

Address : 289 Charoen Nakhon Road, Khlong San, Bangkok 10600, Thailand

Sampling Site : Residences at Mandarin Oriental Bangkok

Sampling by : Test Tech Co., Ltd.

Sampling Date : 04/07/2024

Received Date : 04/07/2024

Report Date : 11/07/2024

Sample Type : Swimming Water

Sampling Method : Grab

Sampling Time : 09:50 AM

Analytical Date : 04 - 09/07/2024

Report No. : R16624/67

Parameters	Unit	Method	TW15346 /67	Standard ^a	Standard ^b
			Swimming Pool-Main		
* Total Viable Count (37°C)	CFU/mL	SM 2023 (9215 B)	< 1 (not found)	< 10	< 10
* Total Coliform Bacteria	/100 mL	Membrane Filtration	not found	-	-
* <i>E. coli</i>	/100 mL	Membrane Filtration	not found	0	0
<i>Pseudomonas aeruginosa</i>	/100 mL	SM 2023 (9213 E)	not detected	< 10	< 10
Sample Condition		Observation	Clear		

Remark : 1. SM 2023 : Standard Methods for the Examination of Water and Wastewater, APHA, AWWA & WEF, 24th ed., 2023

2. Test marked " * " on this report are not included in scope of Accreditation

3. a : Standard from Customer

4. b : Standard from Customer

R. Dounghatai

Miss DOUNGHATAI RERMWANICH

Analyst

11/07/2024



Miss ORASA YUBUA

Technical Manager

11/07/2024

Reported results refer to the sample as received only.

Test report shall not be reproduced except in full, without written approved of the laboratory.

The laboratory has been accepted as an accredited laboratory complying with the ISO/IEC 17025

Analysis/Test Report

Customer Name : The Iconsiam Superlux Residence Condominium Juristic Person

Address : 289 Charoen Nakhon Road, Khlong San, Bangkok 10600, Thailand

Sampling Site : Residences at Mandarin Oriental Bangkok

Sample Type : Swimming Water

Sampling by : Test Tech Co., Ltd.

Sampling Method : Grab

Sampling Date : 06/08/2024

Sampling Time : 10:10 AM

Received Date : 07/08/2024

Analytical Date : 07 - 14/08/2024

Report Date : 17/08/2024

Report No. : R19683/67

Parameters	Unit	Method	TW18026 /67	Standard ^a	Standard ^b
			Swimming Pool-Main		
pH (25°C)	-	Based on SM 2023 (4500-H ⁺ B)	7.4	7.2-7.4	7.2-7.4
Dissolved Solids	mg/L as NaCl	Electrical Conductivity	2298	xx	xx
Total Alkalinity	mg/L as CaCO ₃	Titration	10	-	-
Calcium Hardness	mg/L as CaCO ₃	EDTA Titrimetric	84	75-150	75-150
Chloride	mg/L as Cl ⁻	SM 2023 (4500-Cl ⁻ B)	1140	0-600	0-600
Sulfate	mg/L as SO ₄ ²⁻	Based on SM 2023 (4500-SO ₄ ²⁻ E)	9.74	0-200	0-200
Free Chlorine	mg/L as Cl ₂	DPD Colorimetric	1.01	0.5	1.1-2.2
Combine Chlorine	mg/L as Cl ₂	DPD Colorimetric	0.12	x	x
Cyanuric acid	mg/L	Colorimetric	3	50-100	50-100
Bromine	mg/L	DPD Colorimetric	2.34	4.0-6.0	4.0-6.0
Sample Condition		Observation	Clear		

Remark : 1. SM 2023 : Standard Methods for the Examination of Water and Wastewater, APHA, AWWA & WEF, 24th ed., 2023

2. a : Standard from Customer

x : Less than half the free chlorine or 1.0 whichever is less

xx : < 1000 above source water

3. b : Standard from Customer

x : Less than half the free chlorine or 1.0 whichever is less

xx : < 1000 above source water

R. Prangtip

Miss PRANGTIP RAKSASUK

Analyst

17/08/2024



Miss ORASA LTDYUBUA

Technical Manager

17/08/2024

Reported results refer to the sample as received only.

Test report shall not be reproduced except in full, without written approved of the laboratory.

The laboratory has been accepted as an accredited laboratory complying with the ISO/IEC 17025

TESTING
NO.0001

Analysis/Test Report

Customer Name : The Iconsiam Superlux Residence Condominium Juristic Person

Address : 289 Charoen Nakhon Road, Khlong San, Bangkok 10600, Thailand

Sampling Site : Residences at Mandarin Oriental Bangkok

Sample Type : Swimming Water

Sampling by : Test Tech Co., Ltd.

Sampling Method : Grab

Sampling Date : 06/08/2024

Sampling Time : 10:10 AM

Received Date : 07/08/2024

Analytical Date : 07 - 14/08/2024

Report Date : 17/08/2024

Report No. : R19684/67

Parameters	Unit	Method	TW18026 /67	Standard ^a	Standard ^b
			Swimming Pool-Main		
* Total Viable Count (37°C)	CFU/mL	SM 2023 (9215 B)	< 1 (not found)	< 10	< 10
* Total Coliform Bacteria	/100 mL	Membrane Filtration	not found	-	-
* <i>E. coli</i>	/100 mL	Membrane Filtration	not found	0	0
<i>Pseudomonas aeruginosa</i>	/100 mL	SM 2023 (9213 E)	not detected	< 10	< 10
Sample Condition		Observation	Clear		

Remark : 1. SM 2023 : Standard Methods for the Examination of Water and Wastewater, APHA, AWWA & WEF, 24th ed., 2023

2. Test marked " * " on this report are not included in scope of Accreditation

3. a : Standard from Customer

4. b : Standard from Customer

R. Dounghatai

Miss DOUNGHATAI RERMWANICH

Analyst

17/08/2024



Miss GRASATD. YUBUA

Technical Manager

17/08/2024

Reported results refer to the sample as received only.

Test report shall not be reproduced except in full, without written approved of the laboratory.

The laboratory has been accepted as an accredited laboratory complying with the ISO/IEC 17025

Analysis/Test Report

Customer Name : The Iconsiam Superlux Residence Condominium Juristic Person

Address : 289 Charoen Nakhon Road, Khlong San, Bangkok 10600, Thailand

Sampling Site : Residences at Mandarin Oriental Bangkok

Sample Type : Swimming Water

Sampling by : Test Tech Co., Ltd.

Sampling Method : Grab

Sampling Date : 09/09/2024

Sampling Time : 10:15 AM

Received Date : 10/09/2024

Analytical Date : 10 - 16/09/2024

Report Date : 17/09/2024

Report No. : R22607/67

Parameters	Unit	Method	TW20789 /67	Standard ^a	Standard ^b
			Swimming Pool-Main		
pH (25°C)	-	Based on SM 2023 (4500-H ⁺ B)	7.4	7.2-7.4	7.2-7.4
Dissolved Solids	mg/L as NaCl	Electrical Conductivity	2478	xx	xx
Total Alkalinity	mg/L as CaCO ₃	Titration	20	-	-
Calcium Hardness	mg/L as CaCO ₃	EDTA Titrimetric	76	75-150	75-150
Chloride	mg/L as Cl ⁻	SM 2023 (4500-Cl ⁻ B)	1340	0-600	0-600
Sulfate	mg/L as SO ₄ ²⁻	Based on SM 2023 (4500-SO ₄ ²⁻ E)	8.63	0-200	0-200
Free Chlorine	mg/L as Cl ₂	DPD Colorimetric	1.49	0.5	1.1-2.2
Combine Chlorine	mg/L as Cl ₂	DPD Colorimetric	0.40	x	x
Cyanuric acid	mg/L	Colorimetric	3	50-100	50-100
Bromine	mg/L	DPD Colorimetric	2.13	4.0-6.0	4.0-6.0
Sample Condition		Observation	Clear		

Remark : 1. SM 2023 : Standard Methods for the Examination of Water and Wastewater, APHA, AWWA & WEF, 24th ed., 2023

2. a : Standard from Customer

x : Less than half the free chlorine or 1.0 whichever is less

xx : < 1000 above source water

3. b : Standard from Customer

x : Less than half the free chlorine or 1.0 whichever is less

xx : < 1000 above source water

R. Prangtip

Miss PRANGTIP RAKSASUK

Analyst

17/09/2024



17/09/2024

Reported results refer to the sample as received only.

Test report shall not be reproduced except in full, without written approved of the laboratory.

The laboratory has been accepted as an accredited laboratory complying with the ISO/IEC 17025

Analysis/Test Report

Customer Name : The Iconsiam Superlux Residence Condominium Juristic Person

Address : 289 Charoen Nakhon Road, Khlong San, Bangkok 10600, Thailand

Sampling Site : Residences at Mandarin Oriental Bangkok

Sample Type : Swimming Water

Sampling by : Test Tech Co., Ltd.

Sampling Method : Grab

Sampling Date : 09/09/2024

Sampling Time : 10:15 AM

Received Date : 10/09/2024

Analytical Date : 10 - 16/09/2024

Report Date : 17/09/2024

Report No. : R22608/67

Parameters	Unit	Method	TW20789 /67	Standard ^a	Standard ^b
			Swimming Pool-Main		
* Total Viable Count (37°C)	CFU/mL	SM 2023 (9215 B)	< 1 (not found)	< 10	< 10
* Total Coliform Bacteria	/100 mL	Membrane Filtration	not found	-	-
* <i>E. coli</i>	/100 mL	Membrane Filtration	not found	0	0
<i>Pseudomonas aeruginosa</i>	/100 mL	SM 2023 (9213 E)	not detected	< 10	< 10
Sample Condition			Clear		
Observation					

Remark : 1. SM 2023 : Standard Methods for the Examination of Water and Wastewater, APHA, AWWA & WEF, 24th ed., 2023

2. Test marked " * " on this report are not included in scope of Accreditation

3. a : Standard from Customer

4. b : Standard from Customer

R. Dounghatai

Miss DOUNGHATAI RERMWANICH

Analyst

17/09/2024



Miss GRASA YUBUA

Technical Manager

17/09/2024

Reported results refer to the sample as received only.

Test report shall not be reproduced except in full, without written approved of the laboratory.

The laboratory has been accepted as an accredited laboratory complying with the ISO/IEC 17025

Analysis/Test Report

Customer Name : The Iconsiam Superlux Residence Condominium Juristic Person

Address : 289 Charoen Nakhon Road, Khlong San, Bangkok 10600, Thailand

Sampling Site : Residences at Mandarin Oriental Bangkok

Sample Type : Swimming Water

Sampling by : Test Tech Co., Ltd.

Sampling Method : Grab

Sampling Date : 07/10/2024

Sampling Time : 10:20 AM

Received Date : 07/10/2024

Analytical Date : 07 - 11/10/2024

Report Date : 15/10/2024

Report No. : R24790/67

Parameters	Unit	Method	TW22936 /67	Standard ^a	Standard ^b
			Swimming Pool-Main		
pH (25°C)	-	Based on SM 2023 (4500-H ⁺ B)	7.2	7.2-7.4	7.2-7.4
Dissolved Solids	mg/L as NaCl	Electrical Conductivity	2160	xx	xx
Total Alkalinity	mg/L as CaCO ₃	Titration	45	-	-
Calcium Hardness	mg/L as CaCO ₃	EDTA Titrimetric	72	75-150	75-150
Chloride	mg/L as Cl ⁻	SM 2023 (4500-Cl ⁻ B)	990	0-600	0-600
Sulfate	mg/L as SO ₄ ²⁻	Based on SM 2023 (4500-SO ₄ ²⁻ E)	7.32	0-200	0-200
Free Chlorine	mg/L as Cl ₂	DPD Colorimetric	0.88	0.5	1.1-2.2
Combine Chlorine	mg/L as Cl ₂	DPD Colorimetric	0.58	x	x
Cyanuric acid	mg/L	Colorimetric	3	50-100	50-100
Bromine	mg/L	DPD Colorimetric	2.48	4.0-6.0	4.0-6.0
Sample Condition		Observation	Clear		

Remark : 1. SM 2023 : Standard Methods for the Examination of Water and Wastewater, APHA, AWWA & WEF, 24th ed., 2023

2. a : Standard from Customer

x : Less than half the free chlorine or 1.0 whichever is less

xx : < 1000 above source water

3. b : Standard from Customer

x : Less than half the free chlorine or 1.0 whichever is less

xx : < 1000 above source water

R. Prangtip

Miss PRANGTIP RAKSASUK

Analyst

15/10/2024


TEST TECH CO., LTD.
Miss ORASA YUBUA

Technical Manager

15/10/2024

Reported results refer to the sample as received only.

Test report shall not be reproduced except in full, without written approved of the laboratory.

The laboratory has been accepted as an accredited laboratory complying with the ISO/IEC 17025

Analysis/Test Report

Customer Name : The Iconsiam Superlux Residence Condominium Juristic Person

Address : 289 Charoen Nakhon Road, Khlong San, Bangkok 10600, Thailand

Sampling Site : Residences at Mandarin Oriental Bangkok

Sample Type : Swimming Water

Sampling by : Test Tech Co., Ltd.

Sampling Method : Grab

Sampling Date : 07/10/2024

Sampling Time : 10:20 AM

Received Date : 07/10/2024

Analytical Date : 07 - 11/10/2024

Report Date : 15/10/2024

Report No. : R24791/67

Parameters	Unit	Method	TW22936 /67	Standard ^a	Standard ^b
			Swimming Pool-Main		
* Total Viable Count (37°C)	CFU/mL	SM 2023 (9215 B)	< 1 (not found)	< 10	< 10
* Total Coliform Bacteria	/100 mL	Membrane Filtration	not found	-	-
* <i>E. coli</i>	/100 mL	Membrane Filtration	not found	0	0
<i>Pseudomonas aeruginosa</i>	/100 mL	SM 2023 (9213 E)	not detected	< 10	< 10
Sample Condition		Observation	Clear		

Remark : 1. SM 2023 : Standard Methods for the Examination of Water and Wastewater, APHA, AWWA & WEF, 24th ed., 2023

2. Test marked " * " on this report are not included in scope of Accreditation

3. a : Standard from Customer

4. b : Standard from Customer



Miss DOUNGHATAI RERMWANICH

Analyst

15/10/2024



Miss ORASA YUJBUA

Technical Manager

15/10/2024

Reported results refer to the sample as received only.

Test report shall not be reproduced except in full, without written approved of the laboratory.

The laboratory has been accepted as an accredited laboratory complying with the ISO/IEC 17025



Analysis/Test Report

Customer Name : The Iconsiam Superlux Residence Condominium Juristic Person

Address : 289 Charoen Nakhon Road, Khlong San, Bangkok 10600, Thailand

Sampling Site : Residences at Mandarin Oriental Bangkok

Sample Type : Swimming Water

Sampling by : Test Tech Co., Ltd.

Sampling Method : Grab

Sampling Date : 12/11/2024

Sampling Time : 10:00 AM

Received Date : 13/11/2024

Analytical Date : 13 - 18/11/2024

Report Date : 20/11/2024

Report No. : R27781/67

Parameters	Unit	Method	TW25584 /67	Standard ^a	Standard ^b
			Swimming Pool-Main		
pH (25°C)	-	Based on SM 2023 (4500-H ⁺ B)	7.2	7.2-7.4	7.2-7.4
Dissolved Solids	mg/L as NaCl	Electrical Conductivity	1866	xx	xx
Total Alkalinity	mg/L as CaCO ₃	Titration	35	-	-
Calcium Hardness	mg/L as CaCO ₃	EDTA Titrimetric	63	75-150	75-150
Chloride	mg/L as Cl ⁻	SM 2023 (4500-Cl ⁻ B)	890	0-600	0-600
Sulfate	mg/L as SO ₄ ²⁻	Based on SM 2023 (4500-SO ₄ ²⁻ E)	7.39	0-200	0-200
Free Chlorine	mg/L as Cl ₂	DPD Colorimetric	0.80	0.5	1.1-2.2
Combine Chlorine	mg/L as Cl ₂	DPD Colorimetric	0.18	x	x
Cyanuric acid	mg/L	Colorimetric	4	50-100	50-100
Bromine	mg/L	DPD Colorimetric	2.06	4.0-6.0	4.0-6.0
Sample Condition		Observation	Clear		

Remark : 1. SM 2023 : Standard Methods for the Examination of Water and Wastewater, APHA, AWWA & WEF, 24th ed., 2023

2. a : Standard from Customer

x : Less than half the free chlorine or 1.0 whichever is less

xx : < 1000 above source water

3. b : Standard from Customer

x : Less than half the free chlorine or 1.0 whichever is less

xx : < 1000 above source water

R. Prangtip

Miss PRANGTIP RAKSASUK

Analyst

20/11/2024



Miss ORASA YUBUA

TEST TECH CO., LTD.

Technical Manager

20/11/2024

Reported results refer to the sample as received only.

Test report shall not be reproduced except in full, without written approved of the laboratory.

The laboratory has been accepted as an accredited laboratory complying with the ISO/IEC 17025



Analysis/Test Report

Customer Name : The Iconsiam Superlux Residence Condominium Juristic Person

Address : 289 Charoen Nakhon Road, Khlong San, Bangkok 10600, Thailand

Sampling Site : Residences at Mandarin Oriental Bangkok

Sample Type : Swimming Water

Sampling by : Test Tech Co., Ltd.

Sampling Method : Grab

Sampling Date : 12/11/2024

Sampling Time : 10:00 AM

Received Date : 13/11/2024

Analytical Date : 13 - 18/11/2024

Report Date : 20/11/2024

Report No. : R27782/67

Parameters	Unit	Method	TW25584 /67	Standard ^a	Standard ^b
			Swimming Pool-Main		
Total Viable Count (37°C)	CFU/mL	SM 2023 (9215 B)	< 1 (not found)	< 10	< 10
Total Coliform Bacteria	/100 mL	Membrane Filtration	not found	-	-
<i>E. coli</i>	/100 mL	Membrane Filtration	not found	0	0
<i>Pseudomonas aeruginosa</i>	/100 mL	SM 2023 (9213 E)	not detected	< 10	< 10
Sample Condition		Observation	Clear		

Remark : 1. SM 2023 : Standard Methods for the Examination of Water and Wastewater, APHA, AWWA & WEF, 24th ed., 2023

2. Test marked " * " on this report are not included in scope of Accreditation

3. a : Standard from Customer

4. b : Standard from Customer

R. Dounghatai

Miss DOUNGHATAI RERMWANICH

Analyst

20/11/2024



MISS DOUNGHATAI RERMWANICH

Technical Manager

20/11/2024

Reported results refer to the sample as received only.

Test report shall not be reproduced except in full, without written approved of the laboratory.

The laboratory has been accepted as an accredited laboratory complying with the ISO/IEC 17025

Analysis/Test Report

Customer Name : The Iconsiam Superlux Residence Condominium Juristic Person

Address : 289 Charoen Nakhon Road, Khlong San, Bangkok 10600, Thailand

Sampling Site : Residences at Mandarin Oriental Bangkok

Sample Type : Swimming Water

Sampling by : Test Tech Co., Ltd.

Sampling Method : Grab

Sampling Date : 10/12/2024

Sampling Time : 10:00 AM

Received Date : 11/12/2024

Analytical Date : 11 - 14/12/2024

Report Date : 17/12/2024

Report No. : R29927/67

Parameters	Unit	Method	TW27767 /67	Standard ^a	Standard ^b
			Swimming Pool-Main		
pH (25°C)	-	Based on SM 2023 (4500-H ⁺ B)	7.4	7.2-7.4	7.2-7.4
Dissolved Solids	mg/L as NaCl	Electrical Conductivity	2208	xx	xx
Total Alkalinity	mg/L as CaCO ₃	Titration	75	-	-
Calcium Hardness	mg/L as CaCO ₃	EDTA Titrimetric	68	75-150	75-150
Chloride	mg/L as Cl ⁻	SM 2023 (4500-Cl ⁻ B)	1030	0-600	0-600
Sulfate	mg/L as SO ₄ ²⁻	Based on SM 2023 (4500-SO ₄ ²⁻ E)	7.77	0-200	0-200
Free Chlorine	mg/L as Cl ₂	DPD Colorimetric	1.50	0.5	1.1-2.2
Combine Chlorine	mg/L as Cl ₂	DPD Colorimetric	0.10	x	x
Cyanuric acid	mg/L	Colorimetric	6	50-100	50-100
Bromine	mg/L	DPD Colorimetric	2.78	4.0-6.0	4.0-6.0
Sample Condition		Observation	Clear		

Remark : 1. SM 2023 : Standard Methods for the Examination of Water and Wastewater, APHA, AWWA & WEF, 24th ed., 2023

2. a : Standard from Customer

x : Less than half the free chlorine or 1.0 whichever is less

xx : < 1000 above source water

3. b : Standard from Customer

x : Less than half the free chlorine or 1.0 whichever is less

xx : < 1000 above source water

R. Prangtip

Miss PRANGTIP RAKSASUK

Analyst

17/12/2024



Technical Manager

17/12/2024

Reported results refer to the sample as received only.

Test report shall not be reproduced except in full, without written approved of the laboratory.

The laboratory has been accepted as an accredited laboratory complying with the ISO/IEC 17025

Analysis/Test Report

Customer Name : The Iconsiam Superlux Residence Condominium Juristic Person

Address : 289 Charoen Nakhon Road, Khlong San, Bangkok 10600, Thailand

Sampling Site : Residences at Mandarin Oriental Bangkok

Sample Type : Swimming Water

Sampling by : Test Tech Co., Ltd.

Sampling Method : Grab

Sampling Date : 10/12/2024

Sampling Time : 10:00 AM

Received Date : 11/12/2024

Analytical Date : 11 - 14/12/2024

Report Date : 17/12/2024

Report No. : R29928/67

Parameters	Unit	Method	TW27767 /67	Standard ^a	Standard ^b
			Swimming Pool-Main		
* Total Viable Count (37°C)	CFU/mL	SM 2023 (9215 B)	< 1 (not found)	< 10	< 10
* Total Coliform Bacteria	/100 mL	Membrane Filtration	not found	-	-
* <i>E. coli</i>	/100 mL	Membrane Filtration	not found	0	0
<i>Pseudomonas aeruginosa</i>	/100 mL	SM 2023 (9213 E)	not detected	< 10	< 10
Sample Condition		Observation	Clear		

Remark : 1. SM 2023 : Standard Methods for the Examination of Water and Wastewater, APHA, AWWA & WEF, 24th ed., 2023

2. Test marked " * " on this report are not included in scope of Accreditation

3. a : Standard from Customer

4. b : Standard from Customer

R. Daughatai

Miss DOUNGHATAI RERMWANICH

Analyst

17/12/2024



Miss ORASA YUBUA

Technical Manager

17/12/2024

Reported results refer to the sample as received only.

Test report shall not be reproduced except in full, without written approved of the laboratory.

The laboratory has been accepted as an accredited laboratory complying with the ISO/IEC 17025

Analysis/Test Report

Customer Name : The Iconsiam Superlux Residence Condominium Juristic Person

Address : 289 Charoen Nakhon Road, Khlong San, Bangkok 10600, Thailand

Sampling Site : Residences at Mandarin Oriental Bangkok

Sample Type : Swimming Water

Sampling by : Test Tech Co., Ltd.

Sampling Method : Grab

Sampling Date : 04/07/2024

Sampling Time : 09:50 AM

Received Date : 04/07/2024

Analytical Date : 04 - 08/07/2024

Report Date : 11/07/2024

Report No. : R16514/67

Parameters	Unit	Method	TW15348 /67	TW15349 /67	Standard ^a
			Swimming Pool Deep area	Swimming Pool Shallow area	
* Fecal Coliform Bacteria	MPN/100 mL	SM 2023 (9221 E)	< 1.8	< 1.8	-
<i>Staphylococcus aureus</i>	/100 mL	SM 2023 (9213 B)	not detected	not detected	-
Sample Condition			Clear	Clear	
Observation					

Remark : 1. SM 2023 : Standard Methods for the Examination of Water and Wastewater, APHA, AWWA & WEF, 24th ed., 2023

2. Test marked " * " on this report are not included in scope of Accreditation

3. a : Bangkok Metropolitan Administration published in the Royal Government Gazette, Vol.104 ,Part 205,dated October 14,
B.E.2530 (1987)

R. Dounghatai

Miss DOUNGHATAI RERMWANICH

Analyst

11/07/2024


Miss ORASA YUBUA
TEST TECH CO., LTD.

Technical Manager

11/07/2024

Reported results refer to the sample as received only.

Test report shall not be reproduced except in full, without written approved of the laboratory.

The laboratory has been accepted as an accredited laboratory complying with the ISO/IEC 17025



Analysis/Test Report

Customer Name : The Iconsiam Superlux Residence Condominium Juristic Person

Address : 289 Charoen Nakhon Road, Khlong San, Bangkok 10600, Thailand

Sampling Site : Residences at Mandarin Oriental Bangkok

Sample Type : Swimming Water

Sampling by : Test Tech Co., Ltd.

Sampling Method : Grab

Sampling Date : 06/08/2024

Sampling Time : 10:10 AM

Received Date : 07/08/2024

Analytical Date : 07 - 09/08/2024

Report Date : 13/08/2024

Report No. : R19364/67

Parameters	Unit	Method	TW18028 /67	TW18029 /67	Standard ^a
			Swimming Pool Deep area	Swimming Pool Shallow area	
* Fecal Coliform Bacteria	MPN/100 mL	SM 2023 (9221 E)	< 1.8	< 1.8	-
<i>Staphylococcus aureus</i>	/100 mL	SM 2023 (9213 B)	not detected	not detected	-
Sample Condition		Observation	Clear	Clear	

- Remark : 1. SM 2023 : Standard Methods for the Examination of Water and Wastewater, APHA, AWWA & WEF, 24th ed., 2023
2. Test marked " * " on this report are not included in scope of Accreditation
3. a : Bangkok Metropolitan Administration published in the Royal Government Gazette, Vol.104 ,Part 205,dated October 14, B.E.2530 (1987)

R. Dounghatai

Miss DOUNGHATAI RERMWANICH

Analyst

13/08/2024



Miss YUBUA

Technical Manager

13/08/2024

Reported results refer to the sample as received only.

Test report shall not be reproduced except in full, without written approved of the laboratory.

The laboratory has been accepted as an accredited laboratory complying with the ISO/IEC 17025

TESTING
NO.0001

Analysis/Test Report

Customer Name : The Iconsiam Superlux Residence Condominium Juristic Person

Address : 289 Charoen Nakhon Road, Khlong San, Bangkok 10600, Thailand

Sampling Site : Residences at Mandarin Oriental Bangkok

Sample Type : Swimming Water

Sampling by : Test Tech Co., Ltd.

Sampling Method : Grab

Sampling Date : 09/09/2024

Sampling Time : 10:15 AM

Received Date : 10/09/2024

Analytical Date : 10 - 12/09/2024

Report Date : 13/09/2024

Report No. : R22271/67

Parameters	Unit	Method	TW20791 /67	TW20792 /67	Standard ^a
			Swimming Pool Deep area	Swimming Pool Shallow area	
* Fecal Coliform Bacteria	MPN/100 mL	SM 2023 (9221 E)	< 1.8	< 1.8	-
<i>Staphylococcus aureus</i>	/100 mL	SM 2023 (9213 B)	not detected	not detected	-
Sample Condition			Clear	Clear	

Remark : 1. SM 2023 : Standard Methods for the Examination of Water and Wastewater, APHA, AWWA & WEF, 24th ed., 2023

2. Test marked " * " on this report are not included in scope of Accreditation

3. a : Bangkok Metropolitan Administration published in the Royal Government Gazette, Vol.104 ,Part 205,dated October 14,
B.E.2530 (1987)

R. Daughatai

Miss DOUGHATAI RERMWANICH

Analyst

13/09/2024



13/09/2024

Reported results refer to the sample as received only.

Test report shall not be reproduced except in full, without written approved of the laboratory.

The laboratory has been accepted as an accredited laboratory complying with the ISO/IEC 17025

TESTING
NO.0001

Analysis/Test Report

Customer Name : The Iconsiam Superlux Residence Condominium Juristic Person

Address : 289 Charoen Nakhon Road, Khlong San, Bangkok 10600, Thailand

Sampling Site : Residences at Mandarin Oriental Bangkok

Sample Type : Swimming Water

Sampling by : Test Tech Co., Ltd.

Sampling Method : Grab

Sampling Date : 07/10/2024

Sampling Time : 10:20 AM

Received Date : 07/10/2024

Analytical Date : 07 - 10/10/2024

Report Date : 11/10/2024

Report No. : R24588/67

Parameters	Unit	Method	TW22937 /67	TW22938 /67	Standard ^a
			Swimming Pool Deep area	Swimming Pool Shallow area	
* Fecal Coliform Bacteria	MPN/100 mL	SM 2023 (9221 E)	< 1.8	< 1.8	-
<i>Staphylococcus aureus</i>	/100 mL	SM 2023 (9213 B)	not detected	not detected	-
Sample Condition		Observation	Clear	Clear	

- Remark : 1. SM 2023 : Standard Methods for the Examination of Water and Wastewater, APHA, AWWA & WEF, 24th ed., 2023
2. Test marked " * " on this report are not included in scope of Accreditation
3. a : Bangkok Metropolitan Administration published in the Royal Government Gazette, Vol.104 ,Part 205, dated October 14, B.E.2530 (1987)

R. Dounghatai

Miss DOUNGHATAI RERMWANICH

Analyst

11/10/2024



Miss YUBUA

Technical Manager

11/10/2024

Reported results refer to the sample as received only.

Test report shall not be reproduced except in full, without written approved of the laboratory.

The laboratory has been accepted as an accredited laboratory complying with the ISO/IEC 17025



Analysis/Test Report

Customer Name : The Iconsiam Superlux Residence Condominium Juristic Person

Address : 289 Charoen Nakhon Road, Khlong San, Bangkok 10600, Thailand

Sampling Site : Residences at Mandarin Oriental Bangkok

Sample Type : Swimming Water

Sampling by : Test Tech Co., Ltd.

Sampling Method : Grab

Sampling Date : 12/11/2024

Sampling Time : 10:00 AM

Received Date : 13/11/2024

Analytical Date : 13 - 15/11/2024

Report Date : 16/11/2024

Report No. : R27454/67

Parameters	Unit	Method	TW25585 /67	TW25586 /67	Standard ^a
			Swimming Pool Deep area	Swimming Pool Shallow area	
* Fecal Coliform Bacteria	MPN/100 mL	SM 2023 (9221 E)	< 1.8	< 1.8	-
<i>Staphylococcus aureus</i>	/100 mL	SM 2023 (9213 B)	not detected	not detected	-
Sample Condition			Clear	Clear	

Remark : 1. SM 2023 : Standard Methods for the Examination of Water and Wastewater, APHA, AWWA & WEF, 24th ed., 2023

2. Test marked " * " on this report are not included in scope of Accreditation

3. a : Bangkok Metropolitan Administration published in the Royal Government Gazette, Vol.104 ,Part 205,dated October 14, B.E.2530 (1987)

R. Dounghatai

Miss DOUNGHATAI RERMWANICH

Analyst

16/11/2024



16/11/2024

Reported results refer to the sample as received only.

Test report shall not be reproduced except in full, without written approved of the laboratory.

The laboratory has been accepted as an accredited laboratory complying with the ISO/IEC 17025

Analysis/Test Report

Customer Name : The Iconsiam Superlux Residence Condominium Juristic Person

Address : 289 Charoen Nakhon Road, Khlong San, Bangkok 10600, Thailand

Sampling Site : Residences at Mandarin Oriental Bangkok

Sample Type : Swimming Water

Sampling by : Test Tech Co., Ltd.

Sampling Method : Grab

Sampling Date : 10/12/2024

Sampling Time : 10:00 AM

Received Date : 11/12/2024

Analytical Date : 11 - 13/12/2024

Report Date : 14/12/2024

Report No. : R29723/67

Parameters	Unit	Method	TW27768 /67	TW27769 /67	Standard ^a
			Swimming Pool Deep area	Swimming Pool Shallow area	
* Fecal Coliform Bacteria	MPN/100 mL	SM 2023 (9221 E)	< 1.8	< 1.8	-
<i>Staphylococcus aureus</i>	/100 mL	SM 2023 (9213 B)	not detected	not detected	-
Sample Condition			Clear	Clear	

Remark : 1. SM 2023 : Standard Methods for the Examination of Water and Wastewater, APHA, AWWA & WEF, 24th ed., 2023

2. Test marked " * " on this report are not included in scope of Accreditation

3. a : Bangkok Metropolitan Administration published in the Royal Government Gazette, Vol.104 ,Part 205,dated October 14,
B.E.2530 (1987)

R. Dounghatai

Miss DOUNGHATAI RERMWANICH

Analyst

14/12/2024


Y. Orasa
MISS ORASA YUBUA

Technical Manager

14/12/2024

Reported results refer to the sample as received only.

Test report shall not be reproduced except in full, without written approved of the laboratory.

The laboratory has been accepted as an accredited laboratory complying with the ISO/IEC 17025

ภาคผนวก ง

มาตรฐาน



ภาคผนวก ง-1

ประกาศกระทรวงทรัพยากรธรรมชาติและสิ่งแวดล้อม เรื่อง
กำหนดมาตรฐานควบคุมการระบายน้ำทิ้งจากอาคาร ลงวันที่ 7
พฤศจิกายน 2548 ประกาศในราชกิจจานุเบกษาเล่มที่ 122 ตอน
ที่ 125ง วันที่ 29 ธันวาคม 2548 (ประเภท ข)

ประกาศกระทรวงทรัพยากรธรรมชาติและสิ่งแวดล้อม

เรื่อง กำหนดมาตรฐานควบคุมการระบายน้ำทิ้ง

จากอาคารบางประเภทและบางขนาด

โดยที่ได้มีการปฏิรูประบบราชการโดยให้มีการจัดตั้งกระทรวงทรัพยากรธรรมชาติและสิ่งแวดล้อมขึ้นมา และให้โอนภารกิจของกระทรวงวิทยาศาสตร์ เทคโนโลยีและสิ่งแวดล้อม ในส่วนที่เกี่ยวข้องกับพระราชบัญญัติส่งเสริมและรักษาคุณภาพสิ่งแวดล้อมแห่งชาติ พ.ศ. ๒๕๓๕ ไปเป็นของกระทรวงทรัพยากรธรรมชาติและสิ่งแวดล้อม ประกอบกับเป็นการสมควรให้คณะกรรมการควบคุมมลพิษ เป็นผู้พิจารณาเห็นชอบกับวิธีการตรวจหาค่ามาตรฐานการระบายน้ำทิ้ง นอกเหนือจากวิธีการที่กำหนดไว้ แทนกรมควบคุมมลพิษ จึงสมควรแก้ไขปรับปรุงประกาศกระทรวงวิทยาศาสตร์ เทคโนโลยีและสิ่งแวดล้อม เรื่อง กำหนดมาตรฐานควบคุมการระบายน้ำทิ้งจากอาคารบางประเภทและบางขนาด

อาศัยอำนาจตามความในมาตรา ๕๕ แห่งพระราชบัญญัติส่งเสริมและรักษาคุณภาพสิ่งแวดล้อมแห่งชาติ พ.ศ. ๒๕๓๕ แก้ไขโดยมาตรา ๑๑๔ แห่งพระราชกฤษฎีกาแก้ไขบทบัญญัติให้สอดคล้องกับการโอนอำนาจหน้าที่ของส่วนราชการ ให้เป็นไปตามพระราชบัญญัติปรับปรุงกระทรวง ทบวง กรม พ.ศ. ๒๕๔๕ พ.ศ. ๒๕๔๕ อันเป็นพระราชบัญญัติที่มีบทบัญญัติบางประการเกี่ยวกับการจำกัดสิทธิและเสรีภาพของบุคคล ซึ่งมาตรา ๒๕ ประกอบกับมาตรา ๓๕ มาตรา ๔๘ มาตรา ๕๐ และมาตรา ๕๑ ของรัฐธรรมนูญแห่งราชอาณาจักรไทยบัญญัติให้กระทำได้ โดยอาศัยอำนาจตามบทบัญญัติแห่งกฎหมาย รัฐมนตรีว่าการกระทรวงทรัพยากรธรรมชาติและสิ่งแวดล้อม โดยคำแนะนำของคณะกรรมการควบคุมมลพิษ และโดยความเห็นชอบของคณะกรรมการสิ่งแวดล้อมแห่งชาติ จึงออกประกาศไว้ ดังต่อไปนี้

ข้อ ๑ ให้ยกเลิกประกาศกระทรวงวิทยาศาสตร์ เทคโนโลยีและสิ่งแวดล้อม เรื่อง กำหนดมาตรฐานควบคุมการระบายน้ำทิ้งจากอาคารบางประเภทและบางขนาด ลงวันที่ ๑๐ มกราคม พ.ศ. ๒๕๓๗

ข้อ ๒ ในประกาศนี้

“อาคาร” หมายความว่า อาคารที่ก่อสร้างขึ้น ไม่ว่าจะมิลักษณะเป็นอาคารหลังเดียว หรือเป็นกลุ่มของอาคารซึ่งตั้งอยู่ภายในพื้นที่ซึ่งเป็นบริเวณเดียวกัน และไม่ว่าจะมีท่อระบายน้ำท่อเดียว หรือมีหลายท่อที่เชื่อมติดต่อกันระหว่างอาคารหรือไม่ก็ตาม ซึ่งได้แก่

(๑) อาคารชุด ตามกฎหมายว่าด้วยอาคารชุด

(๒) โรงแรม ตามกฎหมายว่าด้วยโรงแรม

- (๓) หอพัก ตามกฎหมายว่าด้วยหอพัก
- (๔) สถานบริการประเภทสถานอาบน้ำ นวดหรืออบตัว ซึ่งมีผู้ให้บริการแก่ลูกค้า ตามกฎหมายว่าด้วยสถานบริการ
- (๕) โรงพยาบาลของทางราชการหรือสถานพยาบาล ตามกฎหมายว่าด้วยสถานพยาบาล
- (๖) อาคารโรงเรียนเอกชน ตามกฎหมายว่าด้วยโรงเรียนเอกชน โรงเรียนของทางราชการ อาคารสถาบันอุดมศึกษาของเอกชน ตามกฎหมายว่าด้วยสถาบันอุดมศึกษาของเอกชนและสถาบันอุดมศึกษาของทางราชการ
- (๗) อาคารที่ทำการของทางราชการ รัฐวิสาหกิจ หรือองค์การระหว่างประเทศและของเอกชน
- (๘) อาคารของศูนย์การค้าหรือห้างสรรพสินค้า
- (๙) ตลาด ตามกฎหมายว่าด้วยการสาธารณสุข แต่ไม่รวมถึง ท่าเทียบเรือประมง สะพานปลา หรือกิจการแพปลา
- (๑๐) กัฏดาการหรือร้านอาหาร
- “น้ำทิ้ง” หมายความว่า น้ำเสียที่ผ่านระบบบำบัดน้ำเสียแล้วจนเป็นไปตามมาตรฐานควบคุมการระบายน้ำทิ้งตามที่กำหนดไว้ในประกาศนี้
- ข้อ ๓ ให้แบ่งประเภทของอาคารตามข้อ ๒ ออกเป็น ๕ ประเภท คือ
- (๑) อาคารประเภท ก.
- (๒) อาคารประเภท ข.
- (๓) อาคารประเภท ค.
- (๔) อาคารประเภท ง.
- (๕) อาคารประเภท จ.
- ข้อ ๔ อาคารประเภท ก. หมายความว่า อาคารดังต่อไปนี้
- (๑) อาคารชุดที่มีจำนวนห้องสำหรับใช้เป็นที่อยู่อาศัยรวมกันทุกชั้นของอาคาร หรือกลุ่มของอาคาร ตั้งแต่ ๕๐๐ ห้องนอนขึ้นไป
- (๒) โรงแรมที่มีจำนวนห้องสำหรับใช้เป็นห้องพักรวมกันทุกชั้นของอาคาร หรือกลุ่มของอาคาร ตั้งแต่ ๒๐๐ ห้องขึ้นไป
- (๓) โรงพยาบาลของทางราชการ รัฐวิสาหกิจหรือสถานพยาบาล ตามกฎหมายว่าด้วยสถานพยาบาล ที่มีเตียงสำหรับผู้ป่วยไว้ค้างคืนรวมกันทุกชั้นของอาคารหรือกลุ่มของอาคารตั้งแต่ ๓๐ เตียงขึ้นไป

(๔) อาคารโรงเรียนเอกชน โรงเรียนของทางราชการ สถาบันอุดมศึกษาของเอกชน หรือสถาบันอุดมศึกษาของทางราชการที่มีพื้นที่ใช้สอยรวมกันทุกชั้นของอาคารหรือกลุ่มของอาคารตั้งแต่ ๒๕,๐๐๐ ตารางเมตรขึ้นไป

(๕) อาคารที่ทำการของทางราชการ รัฐวิสาหกิจ องค์การระหว่างประเทศ หรือของเอกชน ที่มีพื้นที่ใช้สอยรวมกันทุกชั้นของอาคารหรือกลุ่มของอาคารตั้งแต่ ๕๕,๐๐๐ ตารางเมตรขึ้นไป

(๖) อาคารของศูนย์การค้าหรือห้างสรรพสินค้าที่มีพื้นที่ใช้สอยรวมกันทุกชั้นของอาคารหรือกลุ่มของอาคารตั้งแต่ ๒๕,๐๐๐ ตารางเมตรขึ้นไป

(๗) ตลาดที่มีพื้นที่ใช้สอยรวมกันทุกชั้นของอาคารหรือกลุ่มของอาคารตั้งแต่ ๒,๕๐๐ ตารางเมตรขึ้นไป

(๘) กภัตตาคารหรือร้านอาหารที่มีพื้นที่ให้บริการรวมกันทุกชั้นของอาคารหรือกลุ่มของอาคารตั้งแต่ ๒,๕๐๐ ตารางเมตรขึ้นไป

ข้อ ๕ อาคารประเภท ข. หมายความว่า อาคารดังต่อไปนี้

(๑) อาคารชุดที่มีจำนวนห้องสำหรับใช้เป็นที่อยู่อาศัยรวมกันทุกชั้นของอาคาร หรือกลุ่มของอาคารตั้งแต่ ๑๐๐ ห้องนอน แต่ไม่ถึง ๕๐๐ ห้องนอน

(๒) โรงแรมที่มีจำนวนห้องสำหรับใช้เป็นห้องพักรวมกันทุกชั้นของอาคาร หรือกลุ่มของอาคารตั้งแต่ ๖๐ ห้อง แต่ไม่ถึง ๒๐๐ ห้อง

(๓) หอพักที่มีจำนวนห้องสำหรับใช้เป็นที่อยู่อาศัยรวมกันทุกชั้นของอาคาร หรือกลุ่มของอาคารตั้งแต่ ๒๕๐ ห้องขึ้นไป

(๔) สถานบริการที่มีพื้นที่ใช้สอยรวมกันทุกชั้นของอาคาร หรือกลุ่มของอาคารตั้งแต่ ๕,๐๐๐ ตารางเมตรขึ้นไป

(๕) โรงพยาบาลของทางราชการ รัฐวิสาหกิจ หรือสถานพยาบาล ตามกฎหมายว่าด้วยสถานพยาบาล ที่มีเตียงสำหรับผู้ป่วยไว้ค้างคืนรวมกันทุกชั้นของอาคารหรือกลุ่มของอาคารตั้งแต่ ๑๐ เตียง แต่ไม่ถึง ๓๐ เตียง

(๖) อาคารโรงเรียนเอกชน โรงเรียนของทางราชการ สถาบันอุดมศึกษาของเอกชน หรือสถาบันอุดมศึกษาของทางราชการที่มีพื้นที่ใช้สอยรวมกันทุกชั้นของอาคารหรือกลุ่มของอาคารตั้งแต่ ๕,๐๐๐ ตารางเมตร แต่ไม่ถึง ๒๕,๐๐๐ ตารางเมตร

(๓) อาคารที่ทำการของทางราชการ รัฐวิสาหกิจ องค์การระหว่างประเทศ หรือของเอกชน ที่มีพื้นที่ใช้สอยรวมกันทุกชั้นของอาคารหรือกลุ่มของอาคารตั้งแต่ ๑๐,๐๐๐ ตารางเมตร แต่ไม่ถึง ๕๕,๐๐๐ ตารางเมตร

(๔) อาคารของศูนย์การค้าหรือห้างสรรพสินค้าที่มีพื้นที่ใช้สอยรวมกันทุกชั้นของอาคารหรือกลุ่มของอาคารตั้งแต่ ๕,๐๐๐ ตารางเมตร แต่ไม่ถึง ๒๕,๐๐๐ ตารางเมตร

(๕) ตลาดที่มีพื้นที่ใช้สอยรวมกันทุกชั้นของอาคารหรือกลุ่มของอาคารตั้งแต่ ๑,๕๐๐ ตารางเมตร แต่ไม่ถึง ๒,๕๐๐ ตารางเมตร

(๑๐) กิตติาคารหรือร้านอาหารที่มีพื้นที่ให้บริการรวมกันทุกชั้นของอาคารหรือกลุ่มของอาคาร ตั้งแต่ ๕๐๐ ตารางเมตร แต่ไม่ถึง ๒,๕๐๐ ตารางเมตร

ข้อ ๖ อาคารประเภท ก. หมายความว่า อาคารดังต่อไปนี้

(๑) อาคารชุดที่มีจำนวนห้องสำหรับใช้เป็นที่อยู่อาศัยรวมกันทุกชั้นของอาคาร หรือกลุ่มของอาคาร ไม่ถึง ๑๐๐ ห้องนอน

(๒) โรงแรมที่มีจำนวนห้องสำหรับใช้เป็นที่อยู่พักรวมกันทุกชั้นของอาคาร หรือกลุ่มของอาคาร ไม่ถึง ๖๐ ห้อง

(๓) หอพักที่มีจำนวนห้องสำหรับใช้เป็นที่อยู่อาศัยรวมกันทุกชั้นของอาคาร หรือกลุ่มของอาคาร ตั้งแต่ ๕๐ ห้อง แต่ไม่ถึง ๒๕๐ ห้อง

(๔) สถานบริการที่มีพื้นที่ใช้สอยรวมกันทุกชั้นของอาคาร หรือกลุ่มของอาคารตั้งแต่ ๑,๐๐๐ ตารางเมตร แต่ไม่ถึง ๕,๐๐๐ ตารางเมตร

(๕) อาคารที่ทำการของทางราชการ รัฐวิสาหกิจ องค์การระหว่างประเทศ หรือของเอกชน ที่มีพื้นที่ใช้สอยรวมกันทุกชั้นของอาคารหรือกลุ่มของอาคารตั้งแต่ ๕,๐๐๐ ตารางเมตร แต่ไม่ถึง ๑๐,๐๐๐ ตารางเมตร

(๖) ตลาดที่มีพื้นที่ใช้สอยรวมกันทุกชั้นของอาคารหรือกลุ่มของอาคารตั้งแต่ ๑,๐๐๐ ตารางเมตร แต่ไม่ถึง ๑,๕๐๐ ตารางเมตร

(๗) กิตติาคารหรือร้านอาหารที่มีพื้นที่ให้บริการรวมกันทุกชั้นของอาคาร หรือกลุ่มของอาคาร ตั้งแต่ ๒๕๐ ตารางเมตร แต่ไม่ถึง ๕๐๐ ตารางเมตร

ข้อ ๗ อาคารประเภท ง. หมายความว่า อาคารดังต่อไปนี้

(๑) หอพักที่มีจำนวนห้องสำหรับใช้เป็นที่อยู่อาศัยรวมกันทุกชั้นของอาคาร หรือกลุ่มของอาคาร ตั้งแต่ ๑๐ ห้อง แต่ไม่ถึง ๕๐ ห้อง

(๒) ตลาดที่มีพื้นที่ใช้สอยรวมกันทุกชั้นของอาคาร หรือกลุ่มของอาคารตั้งแต่ ๕๐๐ ตารางเมตร แต่ไม่ถึง ๑,๐๐๐ ตารางเมตร

(๓) กัฏาคารหรือร้านอาหารที่มีพื้นที่ให้บริการรวมกันทุกชั้นของอาคาร หรือกลุ่มของอาคาร ตั้งแต่ ๑๐๐ ตารางเมตร แต่ไม่ถึง ๒๕๐ ตารางเมตร

ข้อ ๘ อาคารประเภท จ. หมายความว่า กัฏาคารหรือร้านอาหารที่มีพื้นที่ให้บริการรวมกันทุกชั้นไม่ถึง ๑๐๐ ตารางเมตร

ข้อ ๙ มาตรฐานควบคุมการระบายน้ำทิ้งจากอาคาร ประเภท ก. ต้องมีค่าดังต่อไปนี้

(๑) ความเป็นกรดและด่าง (PH) ต้องมีค่าระหว่าง ๕-๙

(๒) บีโอดี (BOD) ต้องมีค่าไม่เกิน ๒๐ มิลลิกรัมต่อลิตร

(๓) สารแขวนลอย (Suspended Solids) ต้องมีค่าไม่เกิน ๓๐ มิลลิกรัมต่อลิตร

(๔) ซัลไฟด์ (Sulfide) ต้องมีค่าไม่เกิน ๑.๐ มิลลิกรัมต่อลิตร

(๕) สารที่ละลายได้ทั้งหมด (Total Dissolved Solids) ต้องมีค่าเพิ่มขึ้นจากปริมาณสารละลายในน้ำใช้ตามปกติไม่เกิน ๕๐๐ มิลลิกรัมต่อลิตร

(๖) ตะกอนหนัก (Settleable Solids) ต้องมีค่าไม่เกิน ๐.๕ มิลลิกรัมต่อลิตร

(๗) น้ำมันและไขมัน (Fat Oil and Grease) ต้องมีค่าไม่เกิน ๒๐ มิลลิกรัมต่อลิตร

(๘) ทีเคเอ็น (TKN) ต้องมีค่าไม่เกิน ๓๕ มิลลิกรัมต่อลิตร

ข้อ ๑๐ มาตรฐานควบคุมการระบายน้ำทิ้งจากอาคาร ประเภท ข. ต้องเป็นไปตามข้อ ๙ เว้นแต่

(๑) บีโอดี ต้องมีค่าไม่เกิน ๓๐ มิลลิกรัมต่อลิตร

(๒) สารแขวนลอย ต้องมีค่าไม่เกิน ๔๐ มิลลิกรัมต่อลิตร

ข้อ ๑๑ มาตรฐานควบคุมการระบายน้ำทิ้งจากอาคาร ประเภท ค. ต้องเป็นไปตามข้อ ๙ เว้นแต่

(๑) บีโอดี ต้องมีค่าไม่เกิน ๔๐ มิลลิกรัมต่อลิตร

(๒) สารแขวนลอย ต้องมีค่าไม่เกิน ๕๐ มิลลิกรัมต่อลิตร

(๓) ซัลไฟด์ ต้องมีค่าไม่เกิน ๓.๐ มิลลิกรัมต่อลิตร

(๔) ค่าทีเคเอ็น ต้องมีค่าไม่เกิน ๔๐ มิลลิกรัมต่อลิตร

ข้อ ๑๒ มาตรฐานควบคุมการระบายน้ำทิ้งจากอาคาร ประเภท ง. ต้องเป็นไปตามข้อ ๘
เว้นแต่

(๑) บีโอดี ต้องมีค่าไม่เกิน ๕๐ มิลลิกรัมต่อลิตร

(๒) สารแขวนลอย ต้องมีค่าไม่เกิน ๕๐ มิลลิกรัมต่อลิตร

(๓) ซัลไฟด์ ต้องมีค่าไม่เกิน ๔.๐ มิลลิกรัมต่อลิตร

(๔) ค่าทีเคเอ็น ต้องมีค่าไม่เกิน ๔๐ มิลลิกรัมต่อลิตร

ข้อ ๑๓ มาตรฐานควบคุมการระบายน้ำทิ้งจากอาคาร ประเภท จ. ต้องมีค่าดังต่อไปนี้

(๑) ความเป็นกรดและด่างต้องมีค่าระหว่าง ๕-๙

(๒) บีโอดี ต้องมีค่าไม่เกิน ๒๐๐ มิลลิกรัมต่อลิตร

(๓) สารแขวนลอย ต้องมีค่าไม่เกิน ๖๐ มิลลิกรัมต่อลิตร

(๔) น้ำมันและไขมัน ต้องมีค่าไม่เกิน ๑๐๐ มิลลิกรัมต่อลิตร

ข้อ ๑๔ การตรวจสอบมาตรฐานการระบายน้ำทิ้งจากอาคาร ให้ใช้วิธีการดังต่อไปนี้

(๑) การตรวจสอบค่าความเป็นกรดและด่างให้กระทำโดยใช้เครื่องวัดความเป็นกรดและด่าง
ของน้ำ (PH Meter)

(๒) การตรวจสอบค่าบีโอดีให้กระทำโดยใช้วิธีการอะไซด์โมดิฟิเคชัน (Azide Modification)
ที่อุณหภูมิ ๒๐ องศาเซลเซียส เป็นเวลา ๕ วัน ติดต่อกันหรือวิธีการอื่นที่คณะกรรมการควบคุมมลพิษ
ให้ความเห็นชอบ

(๓) การตรวจสอบค่าสารแขวนลอยให้กระทำโดยใช้วิธีการกรองผ่านกระดาษกรองใยแก้ว
(Glass Fibre Filter Disc)

(๔) การตรวจสอบค่าซัลไฟด์ให้กระทำโดยใช้วิธีการไตเตรท (Titrate)

(๕) การตรวจสอบค่าสารที่ละลายได้ทั้งหมดให้กระทำโดยใช้วิธีการระเหยแห้งระหว่างอุณหภูมิ
๑๐๓ องศาเซลเซียส ถึงอุณหภูมิ ๑๐๕ องศาเซลเซียส ในเวลา ๑ ชั่วโมง

(๖) การตรวจสอบค่าตะกอนหนักให้กระทำโดยใช้วิธีการกรวยอิมฮอฟฟ์ (Imhoff cone)
ขนาดบรรจุ ๑,๐๐๐ ลูกบาศก์เซนติเมตร ในเวลา ๑ ชั่วโมง

(๓) การตรวจสอบค่าน้ำมันและไขมันให้กระทำโดยใช้วิธีการสกัดด้วยตัวทำละลาย แล้วแยกหาน้ำหนักของน้ำมันและไขมัน

(๔) การตรวจสอบค่าที่เคเอ็นให้กระทำโดยใช้วิธีการเจลดาคัล (Kjeldahl)

ข้อ ๑๕ การคิดคำนวณพื้นที่ใช้สอย จำนวนอาคารและจำนวนห้องของอาคาร หรือกลุ่มของอาคาร ให้เป็นไปตามวิธีการที่คณะกรรมการควบคุมมลพิษกำหนด โดยประกาศในราชกิจจานุเบกษา

ข้อ ๑๖ วิธีการเก็บตัวอย่างน้ำ ความถี่ และระยะเวลาในการเก็บตัวอย่างน้ำ ให้เป็นไปตามที่คณะกรรมการควบคุมมลพิษกำหนด โดยประกาศในราชกิจจานุเบกษา

ข้อ ๑๗ ประกาศนี้ให้ใช้บังคับตั้งแต่วันถัดจากวันประกาศในราชกิจจานุเบกษาเป็นต้นไป

ประกาศ ณ วันที่ ๗ พฤศจิกายน พ.ศ. ๒๕๔๘

ยงยุทธ ดิยะไพรัช

รัฐมนตรีว่าการกระทรวงทรัพยากรธรรมชาติและสิ่งแวดล้อม

ภาคผนวก ง-2

ประกาศกระทรวงทรัพยากรธรรมชาติและสิ่งแวดล้อม
เรื่อง กำหนดมาตรฐานควบคุมการระบายน้ำทิ้งจากอาคารบาง
ประเภทและบางขนาด พ.ศ. 2567 ประกาศในราชกิจจานุเบกษา
เล่มที่ 141 ตอนที่ 233 ง วันที่ 27 สิงหาคม พ.ศ. 2567
(ประเภท ข)

ประกาศกระทรวงทรัพยากรธรรมชาติและสิ่งแวดล้อม
เรื่อง กำหนดมาตรฐานควบคุมการระบายน้ำทิ้งจากอาคารบางประเภทและบางขนาด
พ.ศ. ๒๕๖๗

โดยที่เป็นการสมควรปรับปรุงการกำหนดมาตรฐานควบคุมการระบายน้ำทิ้งจากอาคาร ให้เหมาะสมตามความก้าวหน้าในทางวิทยาศาสตร์ เทคโนโลยี และความเปลี่ยนแปลงทางเศรษฐกิจ สังคม ของประเทศ และให้สอดคล้องกับสภาพการณ์ปัจจุบัน

อาศัยอำนาจตามความในมาตรา ๕๕ แห่งพระราชบัญญัติส่งเสริมและรักษาคุณภาพสิ่งแวดล้อมแห่งชาติ พ.ศ. ๒๕๓๕ รัฐมนตรีว่าการกระทรวงทรัพยากรธรรมชาติและสิ่งแวดล้อม โดยคำแนะนำของคณะกรรมการควบคุมมลพิษ และโดยความเห็นชอบของคณะกรรมการสิ่งแวดล้อมแห่งชาติ จึงออกประกาศไว้ ดังต่อไปนี้

ข้อ ๑ ให้ยกเลิกประกาศกระทรวงทรัพยากรธรรมชาติและสิ่งแวดล้อม เรื่อง กำหนดมาตรฐานควบคุมการระบายน้ำทิ้งจากอาคารบางประเภทและบางขนาด ฉบับลงวันที่ ๗ พฤศจิกายน พ.ศ. ๒๕๔๘

ข้อ ๒ ในประกาศนี้

“อาคาร” หมายความว่า อาคารที่ก่อสร้างขึ้น ไม่ว่าจะมียุทธศาสตร์เป็นอาคารหลังเดียวหรือเป็นกลุ่มของอาคารซึ่งตั้งอยู่ภายในพื้นที่ซึ่งเป็นบริเวณเดียวกัน และไม่มียุทธศาสตร์น้ำท่วมหรือมีหลายท่อที่เชื่อมติดต่อกันระหว่างอาคารหรือไม่ก็ตาม

“น้ำทิ้ง” หมายความว่า น้ำที่เกิดจากกิจกรรมของอาคารที่ระบายหรือจะระบายลงสู่แหล่งน้ำสาธารณะหรือออกสู่สิ่งแวดล้อม

ข้อ ๓ ให้แบ่งอาคาร ออกเป็น ๓ ชนิด คือ

ชนิดที่ ๑ อาคารอยู่อาศัย หมายถึง อาคารที่มีวัตถุประสงค์ให้เป็นที่พักอาศัยของบุคคล ทั้งการอยู่อาศัยอย่างถาวรหรือชั่วคราว ได้แก่

(๑) อาคารชุด ตามกฎหมายว่าด้วยอาคารชุด

(๒) หอพัก ตามกฎหมายว่าด้วยหอพัก

(๓) หอพัก ห้องเช่า ห้องแบ่งเช่า หรือกิจการอื่นในทำนองเดียวกันตามกฎหมายว่าด้วยการสาธารณสุข

(๔) สถานรับเลี้ยงเด็ก ตามกฎหมายว่าด้วยคุ้มครองเด็ก

(๕) สถานดูแลผู้สูงอายุหรือผู้มีภาวะพึ่งพิง ตามกฎหมายว่าด้วยสถานประกอบการเพื่อสุขภาพ

(๖) ที่พักอาศัยสำหรับลูกจ้างประเภทกิจกรรมก่อสร้าง ตามกฎหมายว่าด้วยการคุ้มครองแรงงาน

ชนิดที่ ๒ อาคารพาณิชยกรรม หมายถึง อาคารที่ใช้ประโยชน์ในการพาณิชยกรรม หรือบริการธุรกิจ อย่างเดียวหรือหลายอย่าง ได้แก่

(๑) โรงแรม ตามกฎหมายว่าด้วยโรงแรม

- (๒) ศูนย์การค้าหรือห้างสรรพสินค้า
 (๓) ตลาด ตามกฎหมายว่าด้วยการสาธารณสุข
 (๔) สถานบริการประเภทสถานอาบน้ำ นวดหรืออบตัว ตามกฎหมายว่าด้วยสถานบริการ
 (๕) ภัตตาคารหรือร้านอาหาร
 (๖) อาคารที่ทำการของทางราชการ รัฐวิสาหกิจ หรือองค์การระหว่างประเทศและของเอกชน
 (๗) อาคารโรงเรียนเอกชน ตามกฎหมายว่าด้วยโรงเรียนเอกชน โรงเรียนของทางราชการ อาคารสถาบันอุดมศึกษาของเอกชน ตามกฎหมายว่าด้วยสถาบันอุดมศึกษาของเอกชนและสถาบันอุดมศึกษาของทางราชการ

ชนิดที่ ๓ อาคารสถานพยาบาล หมายถึง สถานพยาบาล ตามกฎหมายว่าด้วยสถานพยาบาล ประเภทที่รับผู้ป่วยไว้ค้างคืน

ข้อ ๔ ให้แบ่งขนาดของอาคาร ออกเป็น ๔ ประเภท ดังต่อไปนี้

ประเภทอาคาร	หน่วย	อาคาร ประเภท ก.	อาคาร ประเภท ข.	อาคาร ประเภท ค.	อาคาร ประเภท ง.
๑. อาคารอยู่อาศัย					
อาคารชุด	ห้องชุด	ตั้งแต่ ๕๐๐ ขึ้นไป	ตั้งแต่ ๑๐๐ แต่ไม่ถึง ๕๐๐	ไม่ถึง ๑๐๐	-
หอพัก	ห้อง	-	ตั้งแต่ ๒๕๐ ขึ้นไป	ตั้งแต่ ๕๐ แต่ไม่ถึง ๒๕๐	ไม่ถึง ๕๐
หอพัก ห้องเช่า ห้องแบ่งเช่า หรือกิจการอื่นในทำนอง เดียวกัน ตามกฎหมาย ว่าด้วยการสาธารณสุข	ห้อง	-	ตั้งแต่ ๒๕๐ ขึ้นไป	ตั้งแต่ ๕๐ แต่ไม่ถึง ๒๕๐	ไม่ถึง ๕๐
สถานรับเลี้ยงเด็ก	-	-	-	-	ทุกขนาด
สถานดูแลผู้สูงอายุหรือ ผู้มีภาวะพึ่งพิง	-	-	-	-	ทุกขนาด
ที่พักอาศัยสำหรับลูกจ้าง ประเภทกิจกรรมก่อสร้าง	-	-	-	-	ทุกขนาด
๒. อาคารพาณิชย์					
โรงแรม	ห้อง	ตั้งแต่ ๒๐๐ ขึ้นไป	ตั้งแต่ ๖๐ แต่ไม่ถึง ๒๐๐	ไม่ถึง ๖๐	-
สถานบริการประเภท สถานอาบน้ำ นวดหรืออบตัว	ตาราง เมตร	-	ตั้งแต่ ๕,๐๐๐ ขึ้นไป	ตั้งแต่ ๑,๐๐๐ แต่ไม่ถึง ๕,๐๐๐	ไม่ถึง ๑,๐๐๐
โรงเรียนเอกชน โรงเรียนของ ทางราชการ สถาบันอุดมศึกษา ของเอกชนหรือสถาบัน อุดมศึกษาของทางราชการ		ตั้งแต่ ๒๕,๐๐๐ ขึ้นไป	ตั้งแต่ ๕,๐๐๐ แต่ไม่ถึง ๒๕,๐๐๐	-	ไม่ถึง ๕,๐๐๐

ประเภทอาคาร	หน่วย	อาคาร ประเภท ก.	อาคาร ประเภท ข.	อาคาร ประเภท ค.	อาคาร ประเภท ง.
อาคารที่ทำการของทาง ราชการ รัฐวิสาหกิจ หรือ องค์การระหว่างประเทศและ ของเอกชน		ตั้งแต่ ๕๕,๐๐๐ ขึ้นไป	ตั้งแต่ ๑๐,๐๐๐ แต่ไม่ถึง ๕๕,๐๐๐	ตั้งแต่ ๕,๐๐๐ แต่ไม่ถึง ๑๐,๐๐๐	ไม่ถึง ๕,๐๐๐
ศูนย์การค้า หรือห้างสรรพสินค้า		ตั้งแต่ ๒๕,๐๐๐ ขึ้นไป	ตั้งแต่ ๕,๐๐๐ แต่ไม่ถึง ๒๕,๐๐๐	-	ไม่ถึง ๕,๐๐๐
ตลาด		ตั้งแต่ ๒,๕๐๐ ขึ้นไป	ตั้งแต่ ๑,๕๐๐ แต่ไม่ถึง ๒,๕๐๐	ตั้งแต่ ๑,๐๐๐ แต่ไม่ถึง ๑,๕๐๐	ไม่ถึง ๑,๐๐๐
ภัตตาคารหรือร้านอาหาร		ตั้งแต่ ๒,๕๐๐ ขึ้นไป	ตั้งแต่ ๕๐๐ แต่ไม่ถึง ๒,๕๐๐	ตั้งแต่ ๒๕๐ แต่ไม่ถึง ๕๐๐	ไม่ถึง ๒๕๐
๓. อาคารสถานพยาบาล	เตียง	ตั้งแต่ ๓๐ ขึ้นไป	ตั้งแต่ ๑๐ แต่ไม่ถึง ๓๐	-	ไม่ถึง ๑๐

ข้อ ๕ กำหนดมาตรฐานควบคุมการระบายน้ำทิ้งจากอาคารไว้ ดังต่อไปนี้

พารามิเตอร์	ค่ามาตรฐาน			
	อาคาร ประเภท ก.	อาคาร ประเภท ข.	อาคาร ประเภท ค.	อาคาร ประเภท ง.
๑. ความเป็นกรดและด่าง (pH)	๕.๕ - ๙.๐	๕.๕ - ๙.๐	๕.๕ - ๙.๐	๕.๕ - ๙.๐
๒. บีโอดี (Biochemical Oxygen Demand)	ไม่เกิน ๒๐ มิลลิกรัมต่อลิตร	ไม่เกิน ๓๐ มิลลิกรัมต่อลิตร	ไม่เกิน ๔๐ มิลลิกรัมต่อลิตร	ไม่เกิน ๕๐ มิลลิกรัมต่อลิตร สำหรับอาคารอยู่อาศัย
				ไม่เกิน ๑๐๐ มิลลิกรัมต่อลิตร สำหรับอาคารพาณิชย์ และอาคารสถานพยาบาล
๓. ของแข็งแขวนลอยทั้งหมด (Total Suspended Solids)	ไม่เกิน ๓๐ มิลลิกรัมต่อลิตร	ไม่เกิน ๔๐ มิลลิกรัมต่อลิตร	ไม่เกิน ๕๐ มิลลิกรัมต่อลิตร	ไม่เกิน ๖๐ มิลลิกรัมต่อลิตร
๔. ของแข็งละลายน้ำทั้งหมด (Total Dissolved Solids)	ไม่เกิน ๑,๐๐๐ มิลลิกรัมต่อลิตร	ไม่เกิน ๑,๐๐๐ มิลลิกรัมต่อลิตร	ไม่เกิน ๑,๓๐๐ มิลลิกรัมต่อลิตร	-

พารามิเตอร์	ค่ามาตรฐาน			
	อาคาร ประเภท ก.	อาคาร ประเภท ข.	อาคาร ประเภท ค.	อาคาร ประเภท ง.
	สำหรับอาคารอยู่ อาศัยและอาคาร พาณิชย์	สำหรับอาคารอยู่ อาศัยและอาคาร พาณิชย์	สำหรับอาคารอยู่ อาศัยและอาคาร พาณิชย์	
	เพิ่มขึ้นจาก ปริมาณในน้ำใช้ ปกติไม่เกิน ๑,๐๐๐ สำหรับอาคาร สถานพยาบาล	เพิ่มขึ้นจาก ปริมาณในน้ำใช้ ปกติไม่เกิน ๑,๐๐๐ สำหรับอาคาร สถานพยาบาล	-	-
๕. ซัลไฟด์ (Sulfide)	ไม่เกิน ๑.๐ มิลลิกรัมต่อลิตร	ไม่เกิน ๑.๐ มิลลิกรัมต่อลิตร	ไม่เกิน ๑.๐ มิลลิกรัมต่อลิตร	-
๖. ทีเคเอ็น (Total Kjeldahl Nitrogen)	ไม่เกิน ๓๕ มิลลิกรัมต่อลิตร	ไม่เกิน ๓๕ มิลลิกรัมต่อลิตร	ไม่เกิน ๔๐ มิลลิกรัมต่อลิตร	-
๗. น้ำมันและไขมัน (Oil and Grease)	ไม่เกิน ๒๐ มิลลิกรัมต่อลิตร	ไม่เกิน ๒๐ มิลลิกรัมต่อลิตร	ไม่เกิน ๒๐ มิลลิกรัมต่อลิตร	ไม่เกิน ๒๐ มิลลิกรัมต่อลิตร สำหรับอาคารอยู่อาศัย
				ไม่เกิน ๕๐ มิลลิกรัม ต่อลิตร สำหรับอาคาร พาณิชย์และอาคาร สถานพยาบาล
๘. แบคทีเรียกลุ่มโคลิฟอร์มทั้งหมด (Total Coliform Bacteria) (สำหรับอาคารสถานพยาบาล)	ไม่เกิน ๕,๐๐๐ (เอ็มพีเอ็นต่อ ๑๐๐ มิลลิกรัม)	ไม่เกิน ๕,๐๐๐ (เอ็มพีเอ็นต่อ ๑๐๐ มิลลิกรัม)	-	-
๙. แบคทีเรียกลุ่มฟีคอลโคลิฟอร์ม (Fecal Coliform Bacteria) (สำหรับอาคารสถานพยาบาล)	ไม่เกิน ๑,๐๐๐ (เอ็มพีเอ็นต่อ ๑๐๐ มิลลิกรัม)	ไม่เกิน ๑,๐๐๐ (เอ็มพีเอ็นต่อ ๑๐๐ มิลลิกรัม)	-	-
๑๐. คลอรีนอิสระ (Free Chlorine) (สำหรับอาคารสถานพยาบาล)	ไม่เกิน ๑.๐ มิลลิกรัมต่อลิตร	ไม่เกิน ๑.๐ มิลลิกรัมต่อลิตร	-	-

ข้อ ๖ การตรวจสอบมาตรฐานควบคุมการระบายน้ำทั้งจากอาคารให้ใช้วิธีการ ดังต่อไปนี้

๖.๑ ความเป็นกรดและด่าง ให้ใช้เครื่องวัดความเป็นกรดและด่างของน้ำ (pH Meter) ที่มีความละเอียดไม่ต่ำกว่า ๐.๑ หน่วย

๖.๒ บีโอดี ให้ใช้วิธีบ่มตัวอย่างที่อุณหภูมิ ๒๐ องศาเซลเซียส เป็นเวลา ๕ วันติดต่อกัน และหาค่าออกซิเจนละลายด้วยวิธีเอไซด์มอดิฟิเคชัน (Azide Modification) หรือวิธีเมมเบรนอิเล็กโทรด (Membrane Electrode) หรือวิธีออปติคัลโพรบ (Optical Probe)

๖.๓ ของแข็งแขวนลอยทั้งหมด ให้ใช้วิธีการกรองผ่านกระดาษกรองใยแก้ว (Glass Fiber Filter) และอบแห้งที่อุณหภูมิ ตั้งแต่ ๑๐๓ ถึง ๑๐๕ องศาเซลเซียส เป็นเวลาอย่างน้อย ๑ ชั่วโมง

๖.๔ ของแข็งละลายน้ำทั้งหมด ให้ใช้วิธีระเหยตัวอย่างที่กรองผ่านกระดาษกรองใยแก้ว (Glass Fiber Filter) และอบแห้งที่อุณหภูมิ ๑๘๐ องศาเซลเซียส เป็นเวลาอย่างน้อย ๑ ชั่วโมง

๖.๕ ซัลไฟด์ ให้ใช้วิธีไอโอดิเมทริก (Iodometric Method) หรือวิธีเมทิลีนบลู (Methylene Blue Method)

๖.๖ ทีเคเอ็น ให้ใช้วิธีเจลดาล์ (Kjeldahl)

๖.๗ น้ำมันและไขมัน ให้ใช้วิธีสกัดด้วยตัวทำละลายแล้วแยกหาน้ำหนักของน้ำมันและไขมัน

๖.๘ แบคทีเรียกลุ่มโคลิฟอร์มทั้งหมดและแบคทีเรียกลุ่มฟิคอลโคลิฟอร์ม ให้ใช้วิธีมัลติเพิล ทิวบ์ เฟอ์เมนเทชัน เทคนิค (Multiple Tube Fermentation Technique)

๖.๙ คลอรีนอิสระ ให้ใช้วิธีไทเทรต (Titrimetric method) หรือวิธีเทียบสี (Colorimetric method) หรือวิธีไอโอดิเมทริก อิเล็กโทรด (Iodometric Electrode Technique)

ข้อ ๗ การคิดคำนวณขนาดของอาคารตามข้อ ๔ ให้เป็นไปตามวิธีการที่คณะกรรมการควบคุมมลพิษกำหนด โดยประกาศในราชกิจจานุเบกษา

ข้อ ๘ การตรวจสอบค่ามาตรฐานน้ำทั้งตามข้อ ๖ ต้องเป็นไปตามคู่มือวิเคราะห์น้ำและน้ำเสียของสมาคมวิศวกรรมสิ่งแวดล้อมแห่งประเทศไทย หรือ Standard Methods for the Examination of Water and Wastewater ซึ่ง American Public Health Association, American Water Works Association และ Water Environment Federation ของประเทศสหรัฐอเมริกากำหนดฉบับล่าสุด หรือตามที่คณะกรรมการควบคุมมลพิษประกาศในราชกิจจานุเบกษา

ข้อ ๙ การเก็บตัวอย่างน้ำทั้งเพื่อการตรวจสอบมาตรฐานควบคุมการระบายน้ำทั้งตามข้อ ๕ ให้เป็น ดังต่อไปนี้

๙.๑ ให้เก็บในจุดระบายทิ้งลงสู่แหล่งน้ำสาธารณะหรือออกสู่สิ่งแวดล้อมหรือจุดอื่นที่สามารถใช้เป็นตัวแทนของน้ำทั้งที่ระบายออกจากอาคาร ในกรณีมีการระบายทิ้งหลายจุดให้เก็บทุกจุด

๙.๒ วิธีการเก็บตัวอย่างน้ำทั้ง ณ จุดเก็บตัวอย่างตามข้อ ๙.๑ ให้เก็บแบบจ้วง (Grab Sampling)

ข้อ ๑๐ ประกาศนี้ให้ใช้บังคับตั้งแต่วันถัดจากวันประกาศในราชกิจจานุเบกษาเป็นต้นไป

ประกาศ ณ วันที่ ๒๘ มิถุนายน พ.ศ. ๒๕๖๗

พลตำรวจเอก พัชรวาท วงษ์สุวรรณ

รัฐมนตรีว่าการกระทรวงทรัพยากรธรรมชาติและสิ่งแวดล้อม

ภาคผนวก ง-3

มาตรฐานสรว่ายน้ำ ข้อบังคับกรุงเทพมหานคร
ประกาศในหนังสือราชกิจจานุเบกษาเล่มที่ 104
ตอนที่ 205 ลงวันที่ 14 ตุลาคม 2530

ข้อบังคับกรุงเทพมหานคร

ว่าด้วยหลักเกณฑ์การประกอบการค้าซึ่งเป็นทั้งเรื่อง
หรืออาจเป็นอันตรายแก่สุขภาพประเภทการจัดตั้งสระว่ายน้ำ

พ.ศ. ๒๕๓๐

โดยที่เป็นการสมควรออกข้อบังคับกรุงเทพมหานคร ว่าด้วยหลักเกณฑ์เกี่ยวกับการประกอบการค้าซึ่งเป็นทั้งเรื่องหรืออาจเป็นอันตรายแก่สุขภาพ ประเภทการจัดตั้งสระว่ายน้ำ เพื่อจัดระเบียบควบคุมการประกอบกิจการประเภทนี้ให้เป็นมาตรฐานเดียวกัน มีมาตรการป้องกันเหตุเดือดร้อนรำคาญแก่ประชาชนและอันตรายต่อสุขภาพของผู้ที่เข้าไปใช้บริการ

อาศัยอำนาจตามความในข้อ ๖ และข้อ ๑๔ แห่งข้อบัญญัติกรุงเทพมหานคร เรื่องควบคุมการค้าซึ่งเป็นทั้งเรื่องหรืออาจเป็นอันตรายแก่สุขภาพ พ.ศ. ๒๕๑๕ ผู้ว่าราชการกรุงเทพมหานครจึงออกข้อบังคับไว้ ดังต่อไปนี้

ข้อ ๑ ข้อบังคับนี้เรียกว่า “ข้อบังคับกรุงเทพมหานคร ว่าด้วยหลักเกณฑ์การประกอบการค้าซึ่งเป็นทั้งเรื่องหรืออาจเป็นอันตรายแก่สุขภาพ ประเภทการจัดตั้งสระว่ายน้ำ พ.ศ. ๒๕๓๐”

ข้อ ๒ ข้อบังคับนี้ให้ใช้บังคับตั้งแต่วันถัดจากวันประกาศในราชกิจจานุเบกษาเป็นต้นไป

ข้อ ๓ บรรดาระเบียง ขอบบังคับ ประกาศ หรือคำสั่งอื่นใดที่กำหนดไว้แล้วในขอบบังคับหรือขงัดหรือแย้งกับขอบบังคับ ให้ใช้ขอบบังคับแทน

ข้อ ๔ ในขอบบังคับ

“สระว่ายน้ำ” หมายความว่า สระว่ายน้ำที่เปิดบริการแก่ประชาชนทั่วไป หรือประชาชนเฉพาะกลุ่ม โดยเรียกเก็บค่าบริการ หรือค่าตอบแทนเพื่อการค้า ไม่ว่าโดยตรงหรือโดยอ้อม

“ผู้ใช้บริการ” หมายความว่า ผู้ใช้สระว่ายน้ำ หรือผู้ที่เข้ามาในบริเวณสระว่ายน้ำ

“ผู้ใส่ว่ายน้ำ” หมายความว่า ผู้ที่ลงว่ายน้ำหรือเล่นน้ำในสระว่ายน้ำ

“ส่วนตื้น” หมายความว่า สระว่ายน้ำส่วนที่มีความลึกจากผิวน้ำถึงพื้นสระว่ายน้ำ ไม่มากกว่า ๑.๕๐ เมตร

“ส่วนลึก” หมายความว่า สระว่ายน้ำส่วนที่มีความลึกจากผิวน้ำถึงพื้นสระว่ายน้ำมากกว่า ๑.๕๐ เมตร

“ระบบน้ำหมุนเวียน” หมายความว่า ระบบการปรับปรุงคุณภาพน้ำในสระว่ายน้ำ โดยการนำน้ำผ่านเครื่องบำบัดคุณภาพน้ำแล้วกลับมาใช้

“อาคารประกอบ” หมายความว่า อาคารซึ่งสร้างไว้เพื่อให้ผู้ใช้บริการได้ใช้อาบนำพลัดเปลี่ยนเสื้อผ้า แต่งตัว และเก็บของตลอดจนห้องสุขา และอ่างล้างมือ

“บริเวณสระว่ายน้ำ” หมายความว่า สระว่ายน้ำ รวมตลอดถึงที่ว่างรอบขอบสระว่ายน้ำซึ่งใช้เป็นที่เดิน

ข้อ ๕ ต้องจัดสถานที่ประกอบกิจการสระว่ายน้ำ ดังนี้

๕.๑ ให้มีที่ว่างรอบขอบสระว่ายน้ำเพื่อเป็นที่เดินไม่น้อยกว่า ๑.๐๐ เมตร โดยวัดจากขอบในของสระว่ายน้ำ

๕.๒ ให้มีอาคารประกอบสำหรับให้บริการแก่ผู้ใช้บริการ

๕.๓ ให้มีที่สำหรับล้างเท้าอยู่ตรงทางเข้าบริเวณสระว่ายน้ำ เพื่อให้ผู้ใช้บริการล้างเท้าก่อนเข้าบริเวณสระว่ายน้ำ

๕.๔ ให้มีที่ว่างหรือเก็บรองเท้าของผู้ใช้บริการก่อนเข้าบริเวณสระว่ายน้ำ

ข้อ ๖ สระว่ายน้ำต้องมีลักษณะดังต่อไปนี้

๖.๑ สร้างด้วยคอนกรีตเสริมเหล็กหรือวัสดุที่มีความแข็งแรง น้ำซึมไม่ได้ พื้นและผนังเรียบทำความสะอาดง่าย

๖.๒ มีรางระบายน้ำรอบสระว่ายน้ำ เพื่อรับน้ำล้นที่มีลักษณะทำความสะอาดง่าย และขนาดเพียงพอเพื่อรับน้ำล้น หรือมีบ่อพักน้ำล้น เพื่อให้สามารถรับน้ำล้นเพียงพอ

๖.๓ ขอบสระว่ายน้ำ และทางเดินรอบสระว่ายน้ำต้อง
ไม่ลื่น น้ำไม่ขัง ทำความสะอาดง่ายและสามารถป้องกันน้ำจากทางเดิน
ไหลลงสู่สระว่ายน้ำ

ข้อ ๑ อาคารประกอบต้องมีลักษณะ ดังนี้

๑.๑ อาคารประกอบ ต้องทำด้วยวัสดุมั่นคงแข็งแรง
พื้นเรียบ น้ำซึมไม่ได้ ไม่ลื่น ทำความสะอาดง่าย พื้นลาดเอียงเล็กน้อย
เพื่อการระบายน้ำที่ดี แยกกันเป็นส่วนระหว่างชายและหญิง และ
ต้องจัดให้มีจำนวนสุขภัณฑ์ ดังต่อไปนี้

	หญิง (ที)	ชาย (ที)
ท่อน้ำฝักบัว อย่างน้อย	๒	๒
ส้วม	๒	๒
ทึบส้ววะ	—	๒
อ่างล้างมือ	๒	๒

๑.๒ ให้มีขนาดพื้นที่สะอาดอย่างน้อย ๑ ที ตั้งอยู่ในที่สังเกตเห็นได้ง่าย และต้องรักษาความสะอาดเสมอ

๑.๓ ในกรณีที่ทำการเปิดใช้สระว่ายน้ำในเวลากลางวัน
ต้องจัดให้มีแสงสว่างเพียงพอทั่วบริเวณสระว่ายน้ำ เพื่อให้มองเห็นได้
ชัดเจน

๑.๔ ให้มีตู้เก็บของสำหรับผู้ใส่สระว่ายน้ำ

ข้อ ๘ น้ำในสระว่ายน้ำต้องมีคุณภาพ ดังนี้

๘.๑ น้ำต้องใสสะอาด

๘.๒ ในกรณีที่ใช้คลอรีน น้ำต้องมีปริมาณคลอรีนคง

เหลือไม่น้อยกว่า ๐.๖ มิลลิกรัมต่อลิตรและไม่มากกว่า ๑ มิลลิกรัมต่อลิตร
ในขณะที่มีผู้ใช้สระว่ายน้ำ และต้องมีการเก็บตัวอย่างน้ำเพื่อตรวจหา
ปริมาณคลอรีนคงเหลือทุกวัน แล้วจัดทำเป็นสถิติไว้ให้เจ้าหน้าที่ตรวจ
สอบได้

กรณีที่ใช้ระบบฆ่าเชื้อวิธีอื่น ต้องได้มาตรฐานตามที่กรุงเทพมหานคร
มหานครเห็นสมควร

๘.๓ น้ำต้องมีค่าความเป็นกรด-ด่าง ไม่น้อยกว่า ๗.๒
และไม่มากกว่า ๘.๔ ในขณะที่มีผู้ใช้สระว่ายน้ำ และให้มีการเก็บ
ตัวอย่างน้ำเพื่อตรวจวัดค่าดังกล่าวทุกวัน แล้วจัดทำเป็นสถิติไว้ให้เจ้าหน้าที่
ตรวจสอบได้

๘.๔ คุณสมบัติทางชีววิทยา

๘.๔.๑ ตรวจพบแบคทีเรียชนิดโคลิฟอร์ม (Coliform
Bacteria) น้อยกว่า ๑๐ ต่อน้ำ ๑๐๐ มิลลิลิตร โดยวิธีเอ็มพีเอ็น (Most
Probable Numbers)

๘.๔.๒ ตรวจไม่พบแบคทีเรียชนิด อี. โคไล
(Escherichia coli)

๘.๔.๓ ไม่มีจุลินทรีย์ที่ทำให้เกิดโรค

มีการเก็บตัวอย่างน้ำเพื่อตรวจวิเคราะห์ทางชีววิทยาอย่างน้อยสัปดาห์ที่
ละครั้ง การเก็บตัวอย่างต้องทำอย่างน้อย ๒ จุด คือ ส่วนลึก และส่วนตื้น
ในขณะที่มีผู้ใช้สระว่ายน้ำมากที่สุด แล้วจัดทำเป็นสถิติไว้ให้เจ้าหน้าที่
ตรวจสอบได้

๘.๕ น้าอัตราการหมุนเวียน (Turnover rate) ผ่าน
ระบบน้าหมุนเวียนหมดทั้งสระว่ายน้ำ ภายในเวลาไม่เกิน ๘ ชั่วโมง

ข้อ ๕ การรักษาความสะอาดสระว่ายน้ำ ต้องปฏิบัติดังนี้

๕.๑ จัดให้มีการทำความสะอาดบริเวณสระว่ายน้ำ และ
สำหรับล้างเท้าทุกวันหลังจากปิดการใช้สระว่ายน้ำแล้ว

๕.๒ จัดให้มีเครื่องมือหรืออุปกรณ์สำหรับใช้ทำความสะอาด
สระว่ายน้ำโดยเฉพาะไว้ประจำสระว่ายน้ำ เช่น เครื่องดูดตะกอน
เป็นต้น

๕.๓ ถ้ามองสิ่งสกปรกที่มองเห็นได้ ให้รีบกำจัดออกทันที

๕.๔ จัดให้มีป้ายแสดงกฎ ข้อบังคับสำหรับผู้ใช้สระ
ว่ายน้ำ โดยมีข้อความอย่างน้อย ดังนี้

๕.๔.๑ ต้องสวมชุดว่ายน้ำที่สะอาดในการลงใช้
สระว่ายน้ำ

๕.๔.๒ จำนวนสูงสุดผู้ใช้สระว่ายน้ำ

๕.๔.๓ ต้องชำระล้างร่างกายก่อนลงใช้ส้วมว่ายน้ำ
ทุกครั้ง และห้ามทำส้วมว่ายน้ำสกปรก

๕.๔.๔ ผู้เป็นโรคตาแดง ผื่นหนัง หวัด หูเป็น
น้ำหนอง หรือโรคติดต่ออื่นๆ ห้ามใช้ส้วมว่ายน้ำ

๕.๔.๕ กำหนดเวลาเปิด-ปิด ส้วมว่ายน้ำ

๕.๕ จัดให้มีผู้มีความรู้ความสามารถควบคุมดูแลในการ
ปรับปรุงคุณภาพน้ำในส้วมว่ายน้ำให้อยู่ในมาตรฐาน

๕.๖ จัดให้มีเครื่องมือหรืออุปกรณ์เพื่อตรวจสอบปริมาณ
คลอรีน (ในกรณีที่ใช้คลอรีน) และค่าความเป็นกรด-ด่าง ของน้ำไว้ประจำ
ส้วมว่ายน้ำ

ข้อ ๑๐ ห้ามมิให้น้ำส้วมทุกชนิดเข้าไปในบริเวณส้วมว่ายน้ำและ
หรืออาคารประกอบ

ข้อ ๑๑ การจัดระบบความปลอดภัย ต้องปฏิบัติดังต่อไปนี้

๑๑.๑ ในกรณีที่ใช้คลอรีน การเติมคลอรีนห้ามใช้
วิธีเทผงปูนคลอรีนหรือคลอรีนนําลงในส้วมว่ายน้ำโดยตรงในขณะที่มีผู้ใช้
ส้วมว่ายน้ำ

๑๑.๒ จัดให้มีเจ้าหน้าที่รักษาความปลอดภัย ซึ่งมี
ความชำนาญในการว่ายน้ำ และสามารถให้การปฐมพยาบาลได้ ผลัด
เปลี่ยนกันเพื่อดูแลความปลอดภัยและช่วยเหลือผู้ใช้บริการเมื่อเกิดอุบัติเหตุ
เหตุประจำอยู่ตลอดเวลาที่ส้วมว่ายน้ำเปิดบริการ

๑๑.๓ กระดานกระโดดน้ำ จะต้องเป็นกระดานสำหรับกระโดดน้ำที่ได้มาตรฐาน พื้นกระดานกระโดดต้องปูด้วยแผ่นยางกันลื่น (Corrugated sheet rubber) ความสูงของกระดานกระโดดต้องมีความสัมพันธ์กับความลึกของน้ำบริเวณที่ใช้กระโดดน้ำที่กำหนด คือ

ความสูงของกระดานกระโดดเหนือระดับผิวน้ำ ความลึกของน้ำอย่างน้อย

เมตร	เมตร
๐.๓๐-๐.๕๐	๒.๑๐
๐.๕๐-๑.๕๐	๒.๔๐
๑.๕๐-๒.๔๐	๒.๗๐
๒.๔๐-๓.๐๐	๓.๐๐

ถ้าเป็นสระว่ายน้ำในร่มต้องมีท่างเหนือกระดานสำหรับกระโดดน้ำ ความสูงไม่น้อยกว่า ๔.๐๐ เมตร

๑๑.๔ จัดให้มีห้องปฐมพยาบาลพร้อมชุดปฐมพยาบาลไว้ประจำสระว่ายน้ำ และเปิดประกาศวิธีการปฐมพยาบาลช่วยคนจมน้ำไว้ในบริเวณสระว่ายน้ำ

๑๑.๕ จัดให้มีอุปกรณ์ประจำสระว่ายน้ำ ดังนี้

๑๑.๕.๑ ไม่ช่วยชีวิตหรือวัตถุอื่นใด ยาวไม่น้อยกว่า ๓.๕๐ เมตร มีน้ำหนักเบาอย่างน้อย ๑ อัน วางไว้ที่ปลายคู่ส่วนลึก

๑๑.๕.๒ ห่วงชูชีพ เช่น ยางในรถยนต์ เส้นผ่าศูนย์กลางภายในไม่น้อยกว่า ๑๕ นิ้ว ผูกไว้กับเชือกยาวไม่น้อยกว่าความกว้างของสรว่ายน้ำ

๑๑.๕.๓ โฟมช่วยชีวิต (Kick Board) อย่างน้อย ๒ อัน

๑๑.๕.๔ เครื่องช่วยหายใจ สำหรับเด็กและผู้ใหญ่อย่างน้อยอย่างละ ๑ เครื่อง อุปกรณ์ดังกล่าวต้องวางไว้ในตำแหน่งที่เห็นได้ชัดเจน และนำมาใช้ได้ทันที

๑๑.๖ มีโทรศัพท์สายตรงไว้ใช้ในบริเวณสรว่ายน้ำ และแจ้งหมายเลขของสถานที่สำคัญ ๆ ไว้ เช่น โรงพยาบาล สถานตำรวจ ที่ทำการของการไฟฟ้านครหลวง เป็นต้น

๑๑.๗ แสดงความลึกของสรว่ายน้ำไว้ให้เห็นชัดเจน

ข้อ ๑๒ สรว่ายน้ำที่ก่อนซื้อบังคับใช้บังคับ ผู้ว่าราชการกรุงเทพมหานครมีอำนาจผ่อนผันการปฏิบัติตามข้อบังคับได้ในระยะเวลาที่เห็นสมควร

ประกาศ ณ วันที่ ๒๖ กันยายน ๒๕๓๐

พลตรี จำลอง ศรีเมือง

ผู้ว่าราชการกรุงเทพมหานคร

ภาคผนวก จ
เอกสารสอบเทียบเครื่องมือ



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000-29 FAX. 0-2719-9484



Cert.No.: 24CG750

Page.: 1 of 2

Certificate of Calibration

Equipment :	Auto Burette
Capacity :	25 mL
Serial No. :	-
ID. No. :	6307BU25/01
Manufacturer :	EM
Made in :	Germany
Submitted by :	TEST TECH CO.,LTD. (Head Office) 30, 32 Rama II Soi 63, Rama II Rd. Samaedam, Bangkhunthian, Bangkok 10150
Ambient Temperature :	(20 ± 2.5) °C
Relative Humidity :	(50 ± 10) %
Barometric Pressure :	761 mmHg
Calibration Procedure :	ASTM E 542 - 01
Calibrated by :	Natcha Chayingcheiw

Approved by :

Approved Signatory

- () Ponpan Paipim
(☒) Srisuda Khamtha
() Sa-ngeunkam Wongsu

Issue Date : 19 February 2024

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

A 0063690



Equipment : Auto Burette
Received Date : 12 February 2024
Condition As-Received : Used Item
Calibration Date : 15 February 2024
Reference : 2402-0338DN-1

Cert.No.: 24CG750

Page.: 2 of 2

Condition of this result of calibration

1. Reference Standard Instruments :

<u>Instruments</u>	<u>Model</u>	<u>Serial No.</u>	<u>ID. No.</u>	<u>Certificate No.</u>	<u>Traceability</u>	<u>Due date</u>
1) Balance	XP205DR	1126143764	140RC004	23MM538	TPA	15 Sep 2024
2) Thermo-Hygrograph	THDX-CE	00016540	140EC001	23H1275	TPA	09 June 2024
3) Thermometer	-	0834181	140EC005	23I948	TPA	10 Aug 2024

This certification is traceable to SI Unit

2. The certificate is valid only to the item calibrated on date and place of calibration.

3. True value is converted to true volume at the standard temperature of 20 °C

Calibration result :

Nominal capacity (mL)	Reading (mL)	Std.dev	Uncertainty (± mL)	k Factor
5	5.0209	0.00115	0.0059	2.00
15	15.0065	0.00159	0.0065	2.00
25	25.0012	0.00185	0.0066	2.00

Remark mL = cm³

Std.dev = Standard deviation

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k , providing a level of confidence of approximately 95 %.

-o0o-

a 1202759

Certificate of Calibration

Certificate No. : 67-300495-1

Page : 1 of 2

Submitted by : Test Tech Co.,Ltd. (Head Office)

30, 32 Rama II Soi 63, Rama II Rd., Samaedam, Bangkhunthain, Bangkok 10150

Equipment : Auto Burette

Manufacturer : EM

Class : A

Capacity : 25 ml

Graduation : 0.05 ml

ID No. : 6310BU25/01

Environment : Ambient Temperature : (20 ± 3) °C

Relative Humidity : (50 ± 10) %

Air Pressure : 1003.0 mbar.

Date of Received : 28 August 2024

Date of Calibration : 30 August 2024

Date of Issue : 30 August 2024

Calibrated by : Areerat Sombun

Calibration Method : In-house method CAL-M3001 based on ASTM E 542-22

Reference Standard Instruments : This certification is traceable to the International System of Units

Electronic Balance

ID No.

Cert. No.

Due Date

Traceability

241005

67-200210-4

02 Dec 2024

National Institute of Metrology (Thailand) (NIMT)

Approved by :

(Wipa Tovadee)

Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhaprachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech.cal@yahoo.com, calibratech.cal@hotmail.com

Certificate of Calibration

Certificate No. : 67-300495-1

Page : 2 of 2

Result of Calibration : This result of true Volume is referred to standard temperature at 20 °C

UUC Condition As-Received : Good

Delivery Time : 34.20 sec.


Nominal Volume (ml)	Measuring Volume (ml)
5	4.9776
15	14.9768
25	24.9767

Uncertainty of measurement with in \pm 0.0066 ml

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2.00$,
providing a level of confidence of approximately 95%

- o0o -

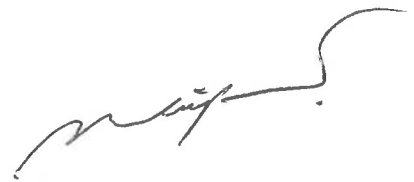

**QUALITY CALIBRATION CO., LTD.**

235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160

Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

www.qcalibration.com



CERTIFICATE No : 24T8053

REFERENCE No : 74209-2

PAGE : 1 OF 3

Certificate of Calibration

EQUIPMENT : BOD INCUBATOR

MANUFACTURER : N/A

MODEL : N/A

SERIAL No : N/A

ID No : EQL-166

CONDITION AS RECEIVED : USED ITEM

SUBMITTED BY : TEST TECH CO., LTD.
30,32 RAMA II SOI 63, RAMA II RD., SAMAEDAM,
BANGKHUNTHIAN, BANGKOK 10150

CALIBRATED BY : CHAICHARN CH.

CALIBRATION DATE : 13-Aug-24

APPROVED BY : 
PONGSAK J.

ISSUED DATE : 19-Aug-24

RECEIVED DATE : 13-Aug-24



QUALITY CALIBRATION CO., LTD.

235 Petchkasem 63/2 Road, Laksong, Bangkai, Bangkok 10160

Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

CERTIFICATE No : 24T8053

PAGE : 2 OF 3

Calibration Report

EQUIPMENT : BOD INCUBATOR
MANUFACTURER : N/A
ID NUMBER : EQL-166
RECEIVED DATE : 13-Aug-24
AMBIENT TEMPERATURE : 25° C ± 1° C
MODEL : N/A
SERIAL NUMBER : N/A
CALIBRATION DATE : 13-Aug-24
RELATIVE HUMIDITY : 54 %RH ± 10 % RH

CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED ACCORDING TO TLAS G-20 BY COMPARISON WITH CALIBRATED THERMOCOUPLE TYPE K UNDER NO LOAD CONDITION. THE THERMOCOUPLES WERE PLACED ON 19 POINTS AND LOCATED AS THE PICTURE BELOW AND WAS AWAY FROM THE EACH WALL OF 5 cm TO 10 cm. AND PLACED THE TENTH THERMOCOUPLE WITHIN 2.5 cm. OF THE GEOMETRIC CENTER OF THE CHAMBER. THE UNIFORMITY WAS MEASURED BETWEEN REFERENCE PROBE AND OTHER PROBES AT THE SAME TIME.

2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) DATA LOGGER WITH TC TYPE K	HYDRA 2635A	7286308	24T6471	24-Jun-25

3. THE CERTIFICATE IS VALID FOR THE ITEM CALIBRATED AS SHOWN ON THE DATE AND PLACE OF CALIBRATION ONLY.
4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.
5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-
- NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH QUALITY CALIBRATION CO., LTD.


RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

GENERAL INFORMATION

Overall Ambient Temperature around the Chamber (°C) variation : 0
Overall Line Voltage (V) variation : 11
Instrument Condition : Normal
Chamber Size (W*L*H): 190*70*174 cm

CHAMBER PERFORMANCE

Calibrate Point (° C)	Average all Located Temp. (° C)	Temperature Stability (±° C)	Temperature Uniformity (° C)	Overall Variation (° C)
20.0	20.09	0.41	0.47	1.0

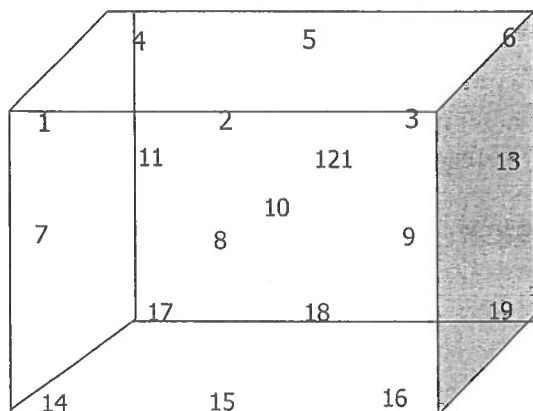

FRONT

END OF CALIBRATION REPORT PAGE 2 OF 3



QUALITY CALIBRATION CO., LTD.

235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160

Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

CERTIFICATE No : 24T8053

PAGE : 3 OF 3

Calibration Report

RESULT OF CALIBRATION (CONTINUE):-

TEMPERATURE MEASUREMENT ACCURACY TEST

Controller temperature (°C)		20.0
Indicating Temperature		20.0
Measured Temperature (°C) at Spread Locations	1	20.00
	2	20.15
	3	20.16
	4	20.17
	5	20.18
	6	20.12
	7	20.21
	8	20.10
	9	20.09
	10 Ref.	19.92
	11	19.97
	12	20.22
	13	20.16
	14	20.11
	15	20.16
	16	20.06
	17	20.01
	18	19.94
	19	20.04
Uncertainty of Measurement(± °C)		0.62

NOTE 1 : THE UNCERTAINTY OF MEASUREMENT EXCLUDED TEMPERATURE UNIFORMITY OF THE CHAMBER.

NOTE 2 : LOCATION 10 WAS REFERENCE LOCATION.

NOTE 3 : THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA.

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR $k=2$, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT



CERTIFICATE No : 24M6587
REFERENCE No : 73767-6

PAGE : 1 OF 2

Certificate of Calibration

EQUIPMENT : DIGITAL BALANCE
MANUFACTURER : SARTORIUS
MODEL : QUINTIX224-1S
SERIAL No : 29302452
ID No : EQL-164
CONDITION AS RECEIVED : USED ITEM
SUBMITTED BY : TEST TECH CO., LTD.
30,32 RAMA II SOI 63, RAMA II RD., SAMAEDAM,
BANGKHUNTHIAN, BANGKOK 10150

CALIBRATED BY : ATSAWIN Y.

CALIBRATION DATE : 01-Jul-24

APPROVED BY : 
PONGSAK J.

ISSUED DATE : 02-Jul-24

RECEIVED DATE : 01-Jul-24



QUALITY CALIBRATION CO.,LTD.

235 Petchkasem 63/2 Road, Laksong, Bangkai, Bangkok 10160

Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

www.qcalibration.com

CERTIFICATE No : 24M6587

PAGE : 2 OF 2

Calibration Report

EQUIPMENT : DIGITAL BALANCE MODEL : QUINTIX224-1S
MANUFACTURER : SARTORIUS S/N : 29302452
ID No : EQL-164 RECEIVED DATE : 01-Jul-24
AIR PRESSURE : 1007mbar \pm 1mbar CALIBRATION DATE : 01-Jul-24
AMBIENT TEMPERATURE : 27° C \pm 1° C RELATIVE HUMIDITY : 55 %RH \pm 10 % RH

CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED BY ACCORDING TO UKAS LAB 14 EDITION 6:2019 BY USING KNOWN WEIGHT STANDARD WEIGHT. THE BALANCE WAS NOT ADJUSTED BEFORE CALIBRATION. THE BALANCE HAS NO ZERO TRACKING FUNCTION. REPEATABILITY WAS MEASURED BY USING 10 REPEATED MEASUREMENTS. LINEARITY WAS MEASURED COVERING 10 POINTS, EVENLY SPREAD OVER THE RANGE. THE INSTRUMENT WAS SET ZERO BEFORE PERFORMING THE LINEARITY TEST. OFF-CENTER LOADING WAS MEASURED BY USING STANDARD WEIGHTS PLACED ON THE PAN AND MOVED TO VARIOUS POSITIONS ON THE PAN.

2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) STANDARD WEIGHT SET	E2	QK-I-151	M2302013S	02-Feb-25
2) STANDARD WEIGHT	E2	15843	M2302014S	02-Feb-25

3. THE CERTIFICATE IS VALID FOR THE ITEM CALIBRATED AS SHOWN ON THE DATE AND PLACE OF CALIBRATION ONLY.

4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.

5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-

- NATIONAL INSTITUTE OF METROLOGY (THAILAND)

RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

1. ZERO SETTING FUNCTION : NORMAL


2. TARE FUNCTION : NORMAL

3. REPEATABILITY OF READING AT 200 g WAS 0.000048 g

4. DEPARTURE FROM NOMINAL VALUE/ LINEARITY

NOMINAL VALUE (g)	BALANCE READING (g)	CORRECTION (g)	UNCERTAINTY (\pm g)
0.0	0.0000	0.0000	0.000096
0.1	0.1000	0.0000	0.000097
0.5	0.5000	0.0000	0.00010
1.0	1.0000	0.0000	0.00010
2.0	2.0000	0.0000	0.00010
20.0	20.0001	-0.0001	0.00011
45.0	45.0001	-0.0001	0.00015
50.0	50.0000	0.0000	0.00013
80.0	80.0001	-0.0001	0.00018
100.0	100.0000	0.0000	0.00019
120.0	120.0000	0.0000	0.00022
140.0	140.0001	-0.0001	0.00025
160.0	160.0000	0.0000	0.00027
180.0	180.0000	0.0000	0.00030
200.0	200.0000	0.0000	0.00032

5. OFF CENTER LOADING ERROR



POINT	READING (g)
1	99.9999
2	99.9999
3	99.9999
4	99.9999
5	100.0000
OFF-CENTER LOADING	0.0001

NOTE: THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA
THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR $k=2$, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT




CERTIFICATE No : 24M6589
REFERENCE No : 73767-8

PAGE : 1 OF 2

Certificate of Calibration

EQUIPMENT : DIGITAL BALANCE
MANUFACTURER : SARTORIUS
MODEL : BCA224i-1S
SERIAL No : 43402017
ID No : EQL-268
CONDITION AS RECEIVED : USED ITEM
SUBMITTED BY : TEST TECH CO., LTD.
30,32 RAMA II SOI 63, RAMA II RD., SAMAEDAM,
BANGKHUNTHIAN, BANGKOK 10150

CALIBRATED BY : ATSAWIN Y.
CALIBRATION DATE : 01-Jul-24

APPROVED BY : 
RONGSAK J.
ISSUED DATE : 02-Jul-24
RECEIVED DATE : 01-Jul-24



QUALITY CALIBRATION CO.,LTD.

235 Petchkasem 63/2 Road, Laksong, Bangkai, Bangkok 10160

Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

www.qcalibration.com

CERTIFICATE No : 24M6589

PAGE : 2 OF 2

Calibration Report

EQUIPMENT : DIGITAL BALANCE
MANUFACTURER : SARTORIUS
ID No : EQL-268
AIR PRESSURE : 1006mbar \pm 1mbar
AMBIENT TEMPERATURE : 25° C \pm 1° C
MODEL : BCA224i-1S
S/N : 43402017
RECEIVED DATE : 01-Jul-24
CALIBRATION DATE : 01-Jul-24
RELATIVE HUMIDITY : 59 %RH \pm 10 % RH

CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED BY ACCORDING TO UKAS LAB 14 EDITION 6:2019 BY USING KNOWN WEIGHT STANDARD WEIGHT. THE BALANCE WAS NOT ADJUSTED BEFORE CALIBRATION. THE BALANCE HAS NO ZERO TRACKING FUNCTION. REPEATABILITY WAS MEASURED BY USING 10 REPEATED MEASUREMENTS. LINEARITY WAS MEASURED COVERING 10 POINTS, EVENLY SPREAD OVER THE RANGE. THE INSTRUMENT WAS SET ZERO BEFORE PERFORMING THE LINEARITY TEST. OFF-CENTER LOADING WAS MEASURED BY USING STANDARD WEIGHTS PLACED ON THE PAN AND MOVED TO VARIOUS POSITIONS ON THE PAN.

2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) STANDARD WEIGHT SET	E2	QK-I-151	M2302013S	02-Feb-25
2) STANDARD WEIGHT	E2	15843	M2302014S	02-Feb-25

3. THE CERTIFICATE IS VALID FOR THE ITEM CALIBRATED AS SHOWN ON THE DATE AND PLACE OF CALIBRATION ONLY.
4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.


5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-
- NATIONAL INSTITUTE OF METROLOGY (THAILAND)

RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

1. ZERO SETTING FUNCTION : NORMAL
2. TARE FUNCTION : NORMAL
3. REPEATABILITY OF READING AT 200 g WAS 0.000042 g
4. DEPARTURE FROM NOMINAL VALUE/ LINEARITY

NOMINAL VALUE (g)	BALANCE READING (g)	CORRECTION (g)	UNCERTAINTY (\pm g)
0.0	0.0000	0.0000	0.000093
0.1	0.1000	0.0000	0.000093
0.5	0.5000	0.0000	0.00009
1.0	1.0000	0.0000	0.00009
2.0	2.0000	0.0000	0.00010
20.0	20.0001	-0.0001	0.00011
45.0	45.0001	-0.0001	0.00015
50.0	50.0000	0.0000	0.00012
80.0	80.0001	-0.0001	0.00018
100.0	100.0000	0.0000	0.00019
120.0	120.0000	0.0000	0.00022
140.0	140.0001	-0.0001	0.00025
160.0	160.0000	0.0000	0.00027
180.0	180.0000	0.0000	0.00030
200.0	200.0000	0.0000	0.00032

5. OFF CENTER LOADING ERROR



POINT	READING (g)
1	100.0000
2	100.0000
3	100.0000
4	100.0000
5	100.0000
OFF-CENTER LOADING	0.0000

NOTE: THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA
THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A
COVERAGE FACTOR $k=2$, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT



CERT.No.: HS-V046G

Harikul Science Co.,Ltd.

694 Soi Ratchadanivet 24, Pracharatbampnen,
Samsaennok, Huaikhwang, Bangkok 10310

Tel: 0-2274-2456 Fax: 0-2274-2443

Email: info@harikul.com www.harikul.com

Certificate of Calibration

Calibration Date : 17 Jul 24

Submitted by : TEST TECH CO.,LTD.

30,32 Ramall Soi 63, Ramall Road, Samaedam,

Bangkhunthian, Bangkok 10150

Avg Room Temp : 20 °C

Avg Water Temp : 20 °C

Air Pressure : 760.00 mmHg

Salinity : 0 ppt

Model : YSI 5000

S/N : 12E102403

Probe : YSI 5010

S/N : 23E100133

ID NO. : EQL-154

Air Temp ref : S/N. F8065C26

Barometric ref : S/N. F8065C26

Water Temp ref : -

ID NO. HS001

Technician : Kittipong M.

Calibration Details

Calibration Point	100% air sat. (@20 °C, DO = 9.09 mg/l)	(status)	(status)	(status)
Measurement 1 (mg/l)	9.08	(PASS)	-	-
Measurement 2 (mg/l)	9.08	(PASS)	-	-
Measurement 3 (mg/l)	9.08	(PASS)	-	-
Measurement 4 (mg/l)	9.08	(PASS)	-	-
Measurement 5 (mg/l)	9.07	(PASS)	-	-
Measurement 6 (mg/l)	9.08	(PASS)	-	-
Measurement 7 (mg/l)	9.07	(PASS)	-	-
Measurement 8 (mg/l)	9.08	(PASS)	-	-
Measurement 9 (mg/l)	9.08	(PASS)	-	-
Measurement 10 (mg/l)	9.08	(PASS)	-	-
Mean Measurement	9.08	mg/l	-	-
Inaccuracy	0.01	mg/l	-	-

Overall Status (PASS)

Manufacturer Specification

Accuracy = +/- 0.02 mg/l

- 1) This certificate is issued based on the result that are found as shown on date and place of test only.
- 2) The calibration procedure followed in accordance with Harikul Science Co., Ltd.
- 3) This result shall not be used for advertising purpose.

Technician Signature
(Kittipong Maekwong)

Laboratory Manager
(Natenapha Pisatkunchon)



QUALITY CALIBRATION CO., LTD.

235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160

Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

www.qcalibration.com

CERTIFICATE No : 24T8911
REFERENCE No : 74483-1

PAGE : 1 OF 2

Certificate of Calibration

EQUIPMENT : HEATING BLOCK
MANUFACTURER : MULBERRY
MODEL : HB-44
SERIAL No : 1904009
ID No : EQL-207
CONDITION AS RECEIVED : USED ITEM
SUBMITTED BY : TEST TECH CO., LTD.
30,32 RAMA II SOI 63, RAMA II RD., SAMAEDAM,
BANGKHUNTHIAN, BANGKOK 10150

CALIBRATED BY : CHAICHARN CH.
CALIBRATION DATE : 05-Sep-24

APPROVED BY : 
PONGSAK J.

ISSUED DATE : 09-Sep-24

RECEIVED DATE : 05-Sep-24





QUALITY CALIBRATION CO., LTD.

235 Petchkasem 63/2 Road, Laksong, Bangkai, Bangkok 10160

Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

CERTIFICATE No : 24T8911

PAGE : 2 OF 2

Calibration Report

EQUIPMENT : HEATING BLOCK
MANUFACTURER : MULBERRY
MODEL : HB-44
ID No : EQL-207
RECEIVED DATE : 05-Sep-24
AMBIENT TEMPERATURE : 26 °C ± 1 °C
S/N : 1904009
CALIBRATION DATE : 05-Sep-24
RELATIVE HUMIDITY : 52 %RH ± 10 %RH


CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED BY DIRECT MEASUREMENT METHOD WITH CALIBRATED RTD PT-100. THE PROBE WERE PLACED ON POINTS AND LOCATED AS THE PICTURE.
2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) DATA LOGGER WITH RTD	HYDRA 2635A	7408027	24T6469	26-Jun-25

3. THE CERTIFICATE IS VALID FOR THE ITEM CALIBRATED AS SHOWN ON THE DATE AND PLACE OF CALIBRATION ONLY.
4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.
5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-
- NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH QUALITY CALIBRATION CO., LTD.

RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

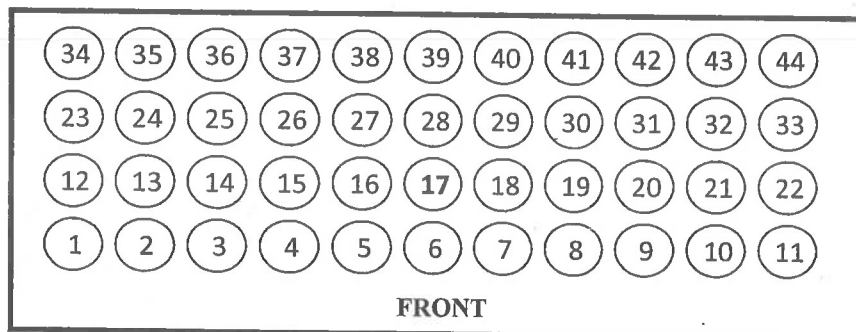

HEATING BLOCK PERFORMANCE

Controller Temperature (°C)	Indicating Temperature (°C)	Temperature Stability (±°C)	Temperature Uniformity (°C)	Overall Variation (°C)
150.0	150.0	0.13	1.59	2.11

TEMPERATURE MEASUREMENT ACCURACY TEST

Measured Temperature (°C) at Spread Locations											Uncertainty (± °C)
1	2	3	4	5	6	7	8	9	10	11	
149.13	149.78	150.38	150.55	150.09	150.89	150.45	150.31	150.65	149.58	149.55	0.82
Measured Temperature (°C) at Spread Locations											Uncertainty (± °C)
12	13	14	15	16	Ref.17	18	19	20	21	22	
149.47	149.96	150.31	149.72	150.77	150.57	150.57	150.91	150.01	149.51	149.66	0.82
Measured Temperature (°C) at Spread Locations											Uncertainty (± °C)
23	24	25	26	27	28	29	30	31	32	33	
149.85	150.16	150.04	150.75	150.63	150.71	151.02	150.36	150.31	150.42	150.25	0.82
Measured Temperature (°C) at Spread Locations											Uncertainty (± °C)
34	35	36	37	38	39	40	41	42	43	44	
149.87	149.70	150.45	150.53	150.76	151.09	150.56	150.06	150.27	150.11	149.71	0.82

NOTE 1: LOCATION 17 WAS REFERENCE LOCATION.

NOTE 2 : THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA.

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR k=2, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT



F-G010 REV : 03



CERTIFICATE No : 24T8915
REFERENCE No : 74483-5

PAGE : 1 OF 2

Certificate of Calibration

EQUIPMENT : HOT AIR OVEN
MANUFACTURER : MEMMERT
MODEL : UFE 500
SERIAL No : G508.0791
ID No : EQL-128
CONDITION AS RECEIVED : USED ITEM
SUBMITTED BY : TEST TECH CO., LTD.
30,32 RAMA II SOI 63, RAMA II RD., SAMAEDAM,
BANGKHUNTHIAN, BANGKOK 10150

CALIBRATED BY : CHAICHARN CH.
CALIBRATION DATE : 05-Sep-24

APPROVED BY : 
PONGSAK J.

ISSUED DATE : 09-Sep-24

RECEIVED DATE : 05-Sep-24





QUALITY CALIBRATION CO., LTD.

235 Petchkasem 63/2 Road, Laksong, Bangkai, Bangkok 10160

Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

CERTIFICATE No : 24T8915

PAGE : 2 OF 2

Calibration Report

EQUIPMENT : HOT AIR OVEN
MANUFACTURER : MEMMERT
MODEL : UFE 500
ID No : EQL-128
RECEIVED DATE : 05-Sep-24
AMBIENT TEMPERATURE : 24 °C ± 1 °C
S/N : G508.0791
CALIBRATION DATE : 05-Sep-24
RELATIVE HUMIDITY : 50 %RH ± 10 %RH

CONDITION OF THIS RESULTS OF CALIBRATION


1. THIS INSTRUMENT WAS CALIBRATED ACCORDING TO TLAS G-20 BY COMPARISON WITH CALIBRATED RTD Pt100 UNDER NO LOAD CONDITION. THE TEMPERATURE PROBES WERE PLACED ON NINE POINTS AND LOCATED ONE THERMOMETER PROBE IN EACH OF THE EIGHT CORNERS OF THE CHAMBER AND WAS AWAY FROM THE EACH WALL OF 5 cm TO 10 cm. AND PLACED THE NINTH THERMOMETER PROBE WITHIN 2.5 cm. OF THE GEOMETRIC CENTER OF THE CHAMBER. THE UNIFORMITY WAS MEASURED BETWEEN REFERENCE PROBE AND OTHER PROBES AT THE SAME TIME.

2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) DATA LOGGER WITH RTD	HYDRA 2635A	6635300	24T6468	26-Jun-25

3. THE CERTIFICATE IS VALID FOR THE ITEM CALIBRATED AS SHOWN ON THE DATE AND PLACE OF CALIBRATION ONLY.
4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.
5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-
- NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH QUALITY CALIBRATION CO., LTD.

RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

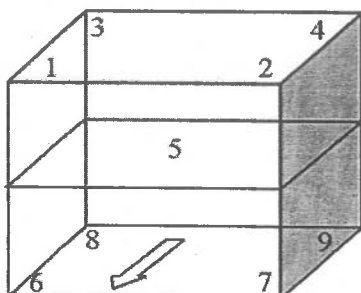

GENERAL INFORMATION

Overall Ambient Temperature around the Chamber (°C) variation : 4
Overall Line Voltage (V) variation : 6
Instrument Condition : Normal
Chamber Size (W*L*H): 56*40*48 cm

CHAMBER PERFORMANCE

Calibrate Point (°C)	Average All Position Temp. (°C)	Temperature Stability (±°C)	Temperature Uniformity (°C)	Overall Variation (°C)
104.0	104.09	0.24	0.72	1.03
180.0	179.88	0.20	1.00	1.24

TEMPERATURE MEASUREMENT ACCURACY TEST

Controller Temp (°C)	Indicating Temp (°C)	Measured Temperature (°C) at Spread Locations									Uncertainty (± °C)
		#1	#2	#3	#4	Ref. 5	#6	#7	#8	#9	
104.0	104.0	104.13	103.69	104.30	103.76	103.78	104.35	104.38	104.13	104.31	0.38
180.0	180.0	180.05	179.34	180.20	179.29	179.51	180.23	180.27	179.92	180.11	1.1

NOTE 1 : THE UNCERTAINTY OF MEASUREMENT EXCLUDED TEMPERATURE UNIFORMITY OF THE CHAMBER.

NOTE 2: LOCATION 5 WAS REFERENCE LOCATION.

NOTE 3 : THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA.

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR k=2, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT



F-G010 REV : 03



CERTIFICATE No : 24T8916
REFERENCE No : 74483-6

PAGE : 1 OF 2

Certificate of Calibration

EQUIPMENT : HOT AIR OVEN
MANUFACTURER : MEMMERT
MODEL : UF 110
SERIAL No : B414.0764
ID No : EQL-169
CONDITION AS RECEIVED : USED ITEM
SUBMITTED BY : TEST TECH CO., LTD.
30,32 RAMA II SOI 63, RAMA II RD., SAMAEDAM,
BANGKHUNTHIAN, BANGKOK 10150

CALIBRATED BY : CHAICHARN CH.

CALIBRATION DATE : 05-Sep-24

APPROVED BY : 
PONGSAK J.

ISSUED DATE : 09-Sep-24

RECEIVED DATE : 05-Sep-24



**QUALITY CALIBRATION CO., LTD.**

235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160

Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

CERTIFICATE No : 24T8916

PAGE : 2 OF 2

Calibration Report

EQUIPMENT : HOT AIR OVEN
 MANUFACTURER : MEMMERT
 MODEL : UF 110
 ID No : EQL-169
 RECEIVED DATE : 05-Sep-24
 AMBIENT TEMPERATURE : 24 °C ± 1 °C

S/N : B414.0764
 CALIBRATION DATE : 05-Sep-24
 RELATIVE HUMIDITY : 50 %RH ± 10 %RH


CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED ACCORDING TO TLAS G-20 BY COMPARISON WITH CALIBRATED RTD Pt100 UNDER NO LOAD CONDITION. THE TEMPERATURE PROBES WERE PLACED ON NINE POINTS AND LOCATED ONE THERMOMETER PROBE IN EACH OF THE EIGHT CORNERS OF THE CHAMBER AND WAS AWAY FROM THE EACH WALL OF 5 cm TO 10 cm. AND PLACED THE NINTH THERMOMETER PROBE WITHIN 2.5 cm. OF THE GEOMETRIC CENTER OF THE CHAMBER. THE UNIFORMITY WAS MEASURED BETWEEN REFERENCE PROBE AND OTHER PROBES AT THE SAME TIME.

2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) DATA LOGGER WITH RTD	HYDRA 2635A	7301307	24T6467	26-Jun-25

3. THE CERTIFICATE IS VALID FOR THE ITEM CALIBRATED AS SHOWN ON THE DATE AND PLACE OF CALIBRATION ONLY.
 4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.
 5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-
 - NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH QUALITY CALIBRATION CO., LTD.

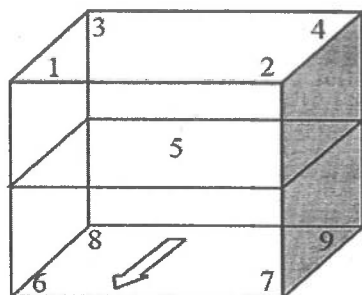RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

FRONT

GENERAL INFORMATION

Overall Ambient Temperature around the Chamber (°C) variation : 3
Overall Line Voltage (V) variation : 8
Instrument Condition : Normal
Chamber Size (W*L*H): 56*40*48 cm

CHAMBER PERFORMANCE

Calibrate Point (°C)	Average All Position Temp. (°C)	Temperature Stability (±°C)	Temperature Uniformity (°C)	Overall Variation (°C)
104.0	104.11	0.06	0.43	0.55
120.0	120.18	0.04	0.58	0.67
140.0	140.24	0.09	0.71	0.91
150.0	150.20	0.10	0.79	0.98

TEMPERATURE MEASUREMENT ACCURACY TEST

Controller Temp (°C)	Indicating Temp (°C)	Measured Temperature (°C) at Spread Locations									Uncertainty (± °C)
		#1	#2	#3	#4	Ref. 5	#6	#7	#8	#9	
104.0	104.0	104.37	104.10	104.39	104.07	104.01	104.25	103.95	103.92	103.97	0.38
120.0	120.0	120.54	120.25	120.45	120.23	120.00	120.33	119.94	119.90	120.00	0.46
140.0	140.0	140.64	140.33	140.53	140.28	139.98	140.48	139.92	139.88	140.09	0.46
150.0	150.0	150.66	150.29	150.55	150.23	149.90	150.47	149.85	149.80	150.06	0.46

NOTE 1 : THE UNCERTAINTY OF MEASUREMENT EXCLUDED TEMPERATURE UNIFORMITY OF THE CHAMBER.

NOTE 2: LOCATION 5 WAS REFERENCE LOCATION.

NOTE 3 : THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA.

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR k =2, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT



F-G010 REV : 03

**QUALITY CALIBRATION CO.,LTD.**

235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160

Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

www.qcalibration.com



CERTIFICATE No : 24T1185

REFERENCE No : 72116-3

PAGE : 1 OF 2

Certificate of Calibration

EQUIPMENT : INCUBATOR

MANUFACTURER : MEMMERT

MODEL : IF 160

SERIAL No : D518.0082

ID No : EQL-205

CONDITION AS RECEIVED : USED ITEM

SUBMITTED BY : TEST TECH CO., LTD.
30,32 RAMA II SOI 63, RAMA II RD., SAMAEDAM,
BANGKHUNTHIAN, BANGKOK 10150

CALIBRATED BY : CHAICHARN CH.

CALIBRATION DATE : 09-Feb-24

APPROVED BY : 
PONGSAK J.

ISSUED DATE : 12-Feb-24

RECEIVED DATE : 09-Feb-24



QUALITY CALIBRATION CO.,LTD.

235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160

Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

CERTIFICATE No : 24T1185

PAGE : 2 OF 2

Calibration Report

EQUIPMENT : INCUBATOR
MANUFACTURER : MEMMERT
MODEL : IF 160
ID No : EQL-205
RECEIVED DATE : 09-Feb-24
AMBIENT TEMPERATURE : 25 °C ± 1 °C
S/N : D518.0082
CALIBRATION DATE : 09-Feb-24
RELATIVE HUMIDITY : 53 %RH ± 10 %RH

CONDITION OF THIS RESULTS OF CALIBRATION


1. THIS INSTRUMENT WAS CALIBRATED ACCORDING TO TLAS G-20 BY COMPARISON WITH CALIBRATED RTD Pt100 UNDER NO LOAD CONDITION. THE TEMPERATURE PROBES WERE PLACED ON NINE POINTS AND LOCATED ONE THERMOMETER PROBE IN EACH OF THE EIGHT CORNERS OF THE CHAMBER AND WAS AWAY FROM THE EACH WALL OF 5 cm TO 10 cm. AND PLACED THE NINTH THERMOMETER PROBE WITHIN 2.5 cm. OF THE GEOMETRIC CENTER OF THE CHAMBER. THE UNIFORMITY WAS MEASURED BETWEEN REFERENCE PROBE AND OTHER PROBES AT THE SAME TIME.

2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) DATA LOGGER WITH RTD	HYDRA 2635A	7301307	23T6636	10-Jul-24

3. THE CERTIFICATE IS VALID FOR THE ITEM CALIBRATED AS SHOWN ON THE DATE AND PLACE OF CALIBRATION ONLY.
4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.
5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-
- NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH QUALITY CALIBRATION CO.,LTD.

RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

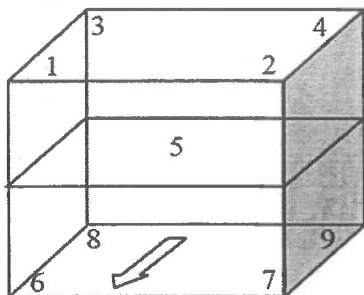

GENERAL INFORMATION

Overall Ambient Temperature around the Chamber (°C) variation : 1
Overall Line Voltage (V) variation : 3
Instrument Condition : Normal
Chamber Size (W*L*H): 56*40*72 cm

CHAMBER PERFORMANCE

Calibrate Point (°C)	Average All Position Temp. (°C)	Temperature Stability (±°C)	Temperature Uniformity (°C)	Overall Variation (°C)
35.0	35.03	0.05	0.09	0.16
36.0	36.05	0.07	0.08	0.19
41.5	41.45	0.08	0.13	0.20

TEMPERATURE MEASUREMENT ACCURACY TEST

Controller Temp (°C)	Indicating Temp (°C)	Measured Temperature (°C) at Spread Locations									Uncertainty (± °C)
		#1	#2	#3	#4	Ref. 5	#6	#7	#8	#9	
35.0	35.0	34.98	35.01	35.00	35.00	35.02	35.08	35.07	35.04	35.10	0.25
36.0	36.0	36.00	36.03	36.03	36.02	36.04	36.09	36.10	36.04	36.12	0.25
41.5	41.5	41.45	41.45	41.39	41.46	41.46	41.47	41.43	41.44	41.49	0.36

NOTE 1 : THE UNCERTAINTY OF MEASUREMENT EXCLUDED TEMPERATURE UNIFORMITY OF THE CHAMBER.

NOTE 2: LOCATION 5 WAS REFERENCE LOCATION.

NOTE 3 : THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA.

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR k=2, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT



CERTIFICATE No : 24E0681
REFERENCE No : 71961-1

PAGE : 1 OF 2

Certificate of Calibration

EQUIPMENT : pH METER
MANUFACTURER : DKK TOA
MODEL : HM-25R
SERIAL No : 760205
ID No : EQL-183
CONDITION AS RECEIVED : USED ITEM
SUBMITTED BY : TEST TECH CO., LTD.
30,32 RAMA II SOI 63, RAMA II RD., SAMAEDAM,
BANGKHUNTHIAN, BANGKOK 10150

CALIBRATED BY : PRASERT D.

CALIBRATION DATE : 23-Jan-24

APPROVED BY : 
PONGSAK J.

ISSUED DATE : 24-Jan-24

RECEIVED DATE : 23-Jan-24

**QUALITY CALIBRATION CO.,LTD.**

235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160

Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

CERTIFICATE No : 24E0681

PAGE : 2 OF 2

Calibration Report

EQUIPMENT : pH METER
MANUFACTURER : DKK TOA
ID No : EQL-183
RECEIVED DATE : 23-Jan-24
AMBIENT TEMPERATURE : 25° C ± 1° C

MODEL : HM-25R
SERIAL NUMBER : 760205
CALIBRATION DATE : 23-Jan-24
RELATIVE HUMIDITY : 50 %RH ± 10 % RH

CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED BY DIRECT MEASUREMENT METHOD BASED ON WI-TQ-062 AND WI-TQ-063. THE DISPLAY UNIT WAS TESTED BY GENERATING STANDARD VOLTAGE TO THE UNIT AND READ THE VALUE COMPARED WITH CALCULATED VALUE. THE DISPLAY AND ELECTROD WAS CALIBRATED BY USING STANDARD pH BUFFER SOLUTION.

2. REFERENCE STANDARD INSTRUMENTS :-

<u>INSTRUMENT</u>	<u>MODEL</u>	<u>SERIAL No/ LOT No</u>	<u>CERTIFICATE No</u>	<u>DUE DATE</u>
1) pH STANDARD SOLUTION	00651-06	CC767907	4880-13836406	29-Dec-24
2) pH STANDARD SOLUTION	00651-08	CC765602	4881-13757019	18-Nov-24
3) pH STANDARD SOLUTION	00651-10	CC767180	4882-13813369	14-Dec-24
4) PROCESS CALIBRATOR	CA150	91S6079	23E1312	19-Apr-24
5) BATH	260014	1247 48074	23T9014	13-Sep-24
6) THERMOMETER WITH PROBE	421504	55000379	23T9623	13-Sep-24

3. THE CERTIFICATE IS VALID FOR THE ITEM CALIBRATED AS SHOWN ON THE DATE AND PLACE OF CALIBRATION ONLY.

4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.

5. THIS CERTIFICATE IS TRACEABLE TO SI UNIT MAINTAINED AT :-

- NATIONAL INSTITUTE OF STANDARD AND TECHNOLOGY, USA.

- NATIONAL INSTITUTE OF METROLOGY (THAILAND)

RESULT OF CALIBRATION : WITHOUT ADJUSTMENT

1. DISPLAY UNIT ONLY

SLOPE FACTOR $k = 2.303 RT/F = 59 \text{ mV/pH}$

mV APPLIED	UUC READING (mV)	CORRECTION (mV)	UNCERTAINTY OF MEASUREMENT (± mV)	COVERAGE FACTOR k
177.48	178	-0.52	0.59	2.0
0.00	1	-1.00	0.59	2.0
-177.48	-177	-0.48	0.59	2.0

2. DISPLAY UNIT WITH pH ELECTRODE S/N: 202F0138MK

STANDARD pH BUFFER SOLUTION (pH)	UUC READING (pH)	CORRECTION (pH)	UNCERTAINTY OF MEASUREMENT (± pH)	COVERAGE FACTOR k
4.0061	4.01	-0.004	0.013	2.0
6.9994	7.00	-0.001	0.013	2.0
10.0070	10.01	-0.003	0.014	2.0

3. PERCENT SLOPE 97%

4. DISPLAY UNIT MEASUREMENT TEMPERATURE WITH PROBE

STANDARD READING (°C)	UUC* READING (°C)	IMMERSION DEPTH (mm)	CORRECTION (°C)	UNCERTAINTY OF MEASUREMENT (±°C)
24.999	25.0	80	-0.001	0.21

UUC : UNIT UNDER CALIBRATION

THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA.

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR k, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT

F-G010 REV 03

การดูแลบำรุงรักษาเชิงป้องกัน

Preventive Maintenance



บริษัท ดีเคเอสเอช เทคโนโลยี จำกัด

ฝ่ายบริการหลังการขาย

โทร 0 2 639 7000 E-mail: service.tec.th@dksh.com

ฝ่ายขายและการตลาด

โทร 0 2 639 7000 E-Mail : marketing.tec.th@dksh.com

Website : www.dksh.co.th/technology/scientific-thailand

เงื่อนไขการให้บริการ Preventive Maintenance

บริษัทฯ จะส่งวิศวกรผู้ชำนาญ เพื่อให้บริการตามขอบข่ายของการบริการ เฉพาะ ในวันและเวลา ราชการ หากมีความประสงค์ที่จะรับบริการนอกเหนือจากวัน เวลา ราชการ (วันหยุดเสาร์ – อาทิตย์ หรือวันหยุด นักชดถุภย์) บริษัท ฯ จะคิดค่าบริการเพิ่มเติมตามอัตราที่กฎหมายแรงงานกำหนดไว้

ขอบข่ายการบริการ

- ตรวจสอบสภาพการทำงานต่าง ๆ ของเครื่องมือ
- ทดสอบประสิทธิภาพการทำงานของเครื่องมือ
- รายการผลการตรวจสอบเครื่องมือ

หมายเหตุ

- ราคานี้ไม่รวมถึงค่าบริการซ่อม หรือ เปลี่ยนอะไหล่ที่ชำรุดเสียหาย หรือหมดสภาพการใช้งาน
- ในกรณีที่ผู้รับบริการอยู่นอกเขตพื้นที่ให้บริการ บริษัทฯ จำเป็นต้องคิดค่าใช้จ่ายเพิ่มเติม ได้แก่ ค่าเดินทาง เป็นต้น
- บริษัท ฯ ขอสงวนสิทธิ์ในการเปลี่ยนแปลงราคา โดยไม่แจ้งให้ทราบล่วงหน้า

ช่องทางการติดต่อ



DKSH Technology Limited (บริษัท ดีเคเอสเอช เทคโนโลยี จำกัด)

เลขที่ 2533 ถนนสุขุมวิท แขวงบางจาก เขตพระโขนง กรุงเทพฯ 10260

เลขประจำตัวผู้เสียภาษี 010-555-001-4547 (สำนักงานใหญ่)



Call center 0 2 639 7000



DKSH Scientific



www.dksh.com/scientific-thailand



marketing.tec.th@dksh.com



@dkshscientific

Preventive Maintenance Contract

จำนวนในการทำสัญญาบริการ ...1...ครั้ง ต่อปี
ครั้งที่ 1 วันที่ 19/04/2024.....

รายละเอียดผู้รับบริการ


หน่วยงาน	บริษัท เทสท์ เทค จำกัด		
ที่อยู่	30,32 ซอยพระรามที่ 2 ซอย 63 ถนนพระรามที่ 2 แขวงสามค่า เขตบางขุนเทียน กรุงเทพมหานคร 10150		
โทรศัพท์	0-2893-4211-7	แฟกซ์	0-2893-4218

ผู้ติดต่อ

ชื่อ - นามสกุล	คุณกรรณก ขุนพิทักษ์				
ตำแหน่ง	หัวหน้าส่วน				
โทรศัพท์	087 398 9274	เบอร์ต่อ	-	แฟกซ์	-
E-mail	lab_center@testtech.co.th				

รายละเอียดผู้ให้บริการ

บริษัท ดีเคเอสเอช เทคโนโลยี จำกัด (ฝ่ายบริการหลังการขาย) (สำนักงานใหญ่) เลขที่ 2533 ถนนสุขุมวิท แขวงบางจาก เขตพระโขนง กรุงเทพฯ 10260 โทรศัพท์ 0 2 693 7000 Email: sudarat.sk@dksh.com เจ้าหน้าที่ประสานงาน : คุณสุดารัตน์ ศิริรัตน์ โทรศัพท์ 090 678 6925	
เจ้าหน้าที่ผู้ให้บริการ	นายจิรายุช สเลอาด
ตำแหน่ง	Specialist, Technical Service.
โทรศัพท์	0938138736 แฟกซ์ -
E-mail	Jirayut.js@dksh.com


ลงนามผู้รับบริการ	กรรณก ขุนพิทักษ์	ลงนามผู้ให้บริการ	
ตัวบรรจง	(นายกรรณก ขุนพิทักษ์)	ตัวบรรจง	(นาย จิรายุช สเลอาด)
ตำแหน่ง	หัวหน้าส่วนทดสอบ	ตำแหน่ง	Specialist, Technical Service.
วันที่ / ประทับตราบริษัท	19/04/2024	วันที่ / ประทับตราบริษัท	19/04/2024

JOB No: LSPR2402440.....MODEL:VAP300.....S/N: GER5300210095

Operational Qualification (OQ)

ตรวจสอบสภาพเครื่อง


FRONT

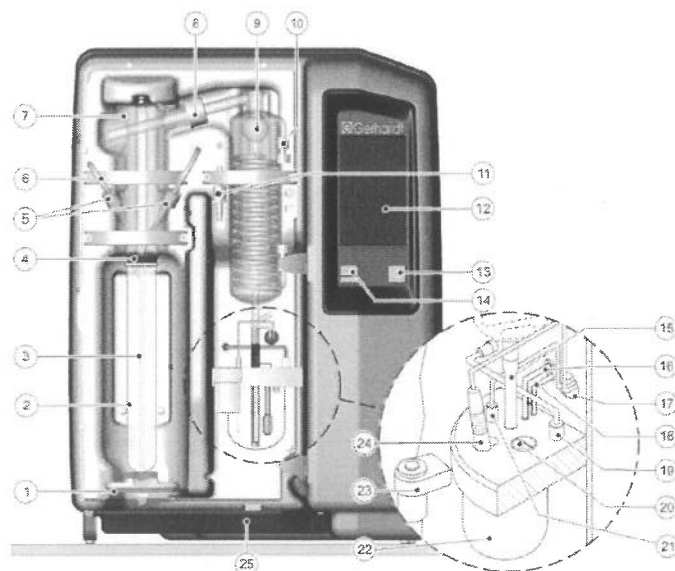

No		PASS	FAIL	N/A
1	Quick clamping device with clamping block	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
2	Digestion tube 250/300 ml	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
3	PTFE steam inlet tubing	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
4	Connection stopper , Viton	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
5	Screw cap GL18	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
6	PTFE-inlet tubing NaOH	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
7	Distribution head made of glass	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
8	Screw cap GL32	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
9	Distillation condenser made of glass	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
10	Screw cap GL14	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
11	Ventilation valve	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
12	Control panel	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
13	Operating Button	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
14	USB interface (with protective cap)	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
15	Silicone tubing 8/10 for distillate discharge **	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>
16	Verprene tubing 4/8 , receiver suction **	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>
17	Cable duct for electrode cable + titration tube**	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>
18	Silicone tubing 4/7 , boric acid inlet**	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>
19	Sensor for level monitoring including connector**	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>
20	Agitator motor with propeller**	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>
21	Titration acid inlet tube **	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>
22	Receiver glass**	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>
23	Holder for pH electrode , removable**	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>
24	pH electrode (combined electrode)**	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>
25	Drip tray PP	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>


** only VAP 450

REAR

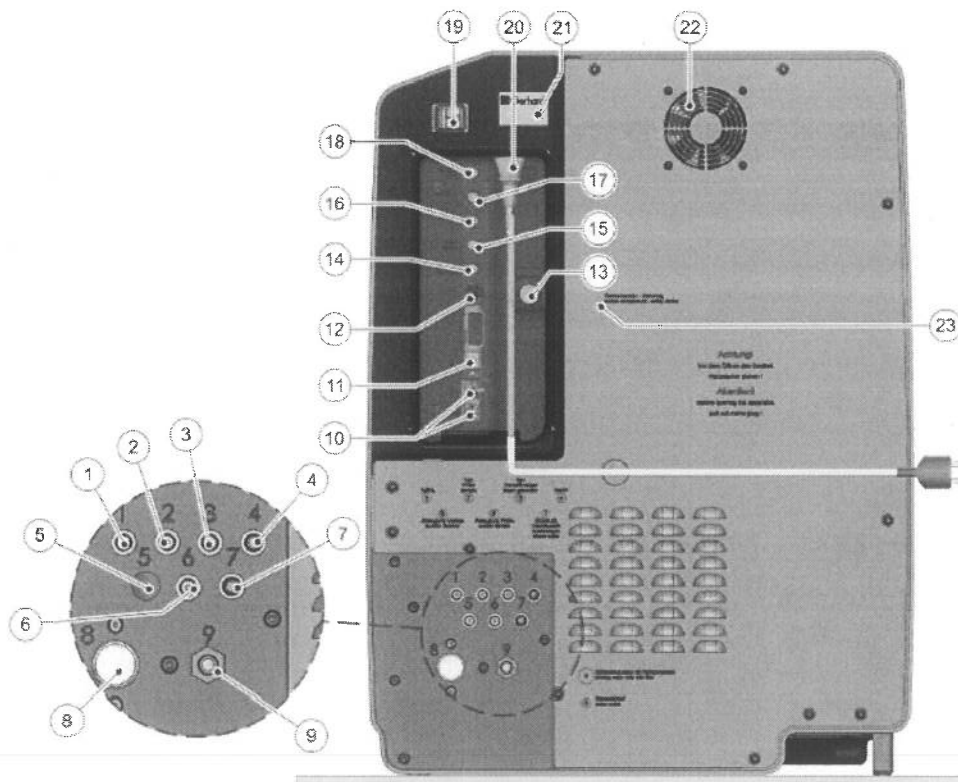


No		PASS	FAIL	N/A
1	Tube connection for sample H3BO3 supply	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>
2	Tube connection for sample H2O supply	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
3	Tube connection for steam generator H2O supply	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
4	Tube connection for NaOH supply	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
5	Tube connection for receiver glass extraction	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
6	Tube connection for sample waste extraction	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
7	Tube connection , overpressure steam outlet	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
8	Connection for cooling water supply (with cleaning sieve)	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
9	Tube connection for cooling water outlet	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
10	4 X USB interface	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
11	1 X RS-232 Interface	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
12	LAN Interface	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
13	Screw cap for Perspex cover	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
14	Connection socket for sample waste tank level monitoring	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
15	Connection (not used)	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>
16	Connection socket for H2O tank level monitoring	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
17	Connection socket for H3BO3 tank level monitoring	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
18	Connection socket for NaOH tank level monitoring	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
19	Overcurrent circuit breaker	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
20	Apparatus socket (mains cable connection)	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
21	Rating plate with serial number	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
22	Exhaust air fan	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
23	Excess temperature switch	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>

Inside Steam generator

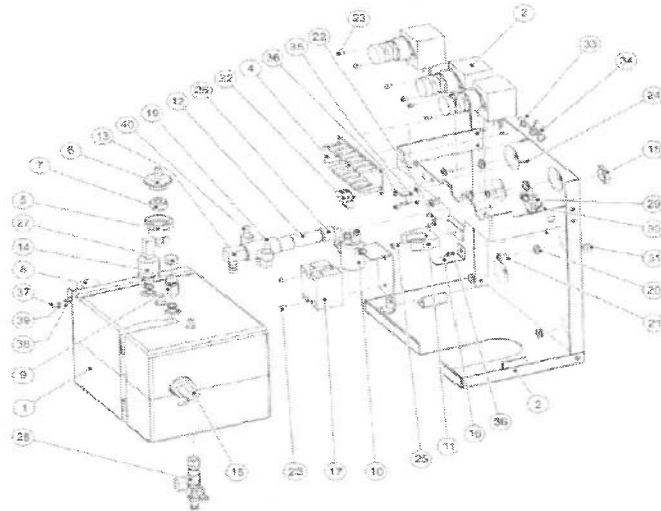


No		PASS	FAIL	N/A
1	Steam generator	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
2	Steam generator traverse	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
3	Pinch valve	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
4	Circuit board distributor	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
5	Valve tubing connection	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
6	Housing safety valve	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
7	Safety valve SKT	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
8	Excess temperature protection , steam generator	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
9	Safety valve G 1/8 0,5 bar	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
10	Ventilation glass pinch valve VAPODEST	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
11	Hose clamp for ventilation clamp	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
12	Distributor PP	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
13	Angle connection PP	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
14	Pressure transmitter	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
15	Level switch	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
16	Fixing bracket steam generator	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
17	Relay HT+	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
18	VA Hexagon nut 1/2"	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
19	Angle connection 1/8"	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
20	Bushing nipple 6-10-14	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
21	VA Lens head screw M5 X 10	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
22	Grounding connection , 2-pole	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
23	VA Lens head screw M4 X 6	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
24	Spacer bolt 5 mm	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
25	VA Lens head screw M4 X 10	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
26	Tubing connection	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
27	Hose clamp 14.5 mm	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
28	Module ball valve with nozzles	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
29	Cross manifold with spout	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
30	Seal copper G 1/8	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
31	Locking screw 1/8"	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
32	Pin strip	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
33	Bundle clamp 12 H 4500	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
34	Bundle clamp 12 H 4502	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
35	Temperature switch 80°C	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
36	VA Lens head screw M3 X 6	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
37	VA Hexagon nut M4	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
38	Lins head screw M4 X 8	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
39	VA Spring washer	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
40	Angle connection , reduced , 1/8" PP	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>

Module Pump holder VAP200 - 450 V3

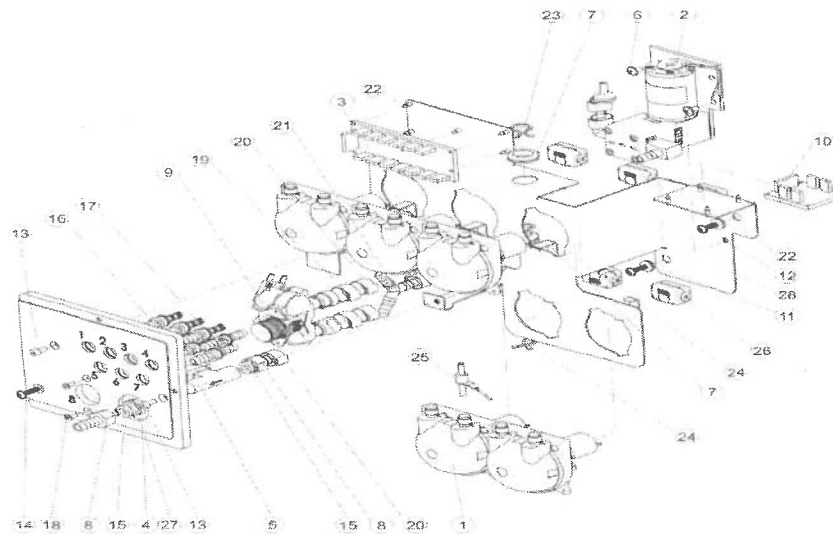

No		PASS	FAIL	N/A
1	Peristaltic pump	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
2	Diaphragm pump NaOH. with non return valve	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
3	Circuit board	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
4	Tubing connection module	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
5	Flow controller	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
6	Lens head screw M5 x 10	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
7	Bushing nozzle	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
8	Screw in socket	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
9	Magnetic valve 2/2 way	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
10	Circuit board distributor	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
11	Bushing nozzle	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
12	Screw 5 x 25	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
13	Cylinder screw	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
14	Screw 5 x 20	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
15	Seal EPDM 15 x 4	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
16	Tubing connection piece 51x10x6,5	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
17	Tubing connection piece 51x10x10	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
18	Screw M4x10	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
19	Clamp	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
20	Clamp	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
21	Y-tube connector	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
22	Spacer bolt 5 mm	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
23	Bundle clamp	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
24	Bundle clamp	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
25	Retrofit earthing pumpv	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
26	Snap ferrite	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
27	Nut G 3/8"	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
28	Pump holder plate	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>

Control panel

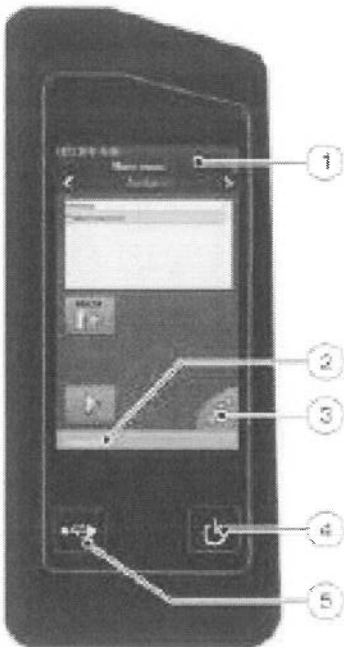

No		PASS	FAIL
1	Title bar	<input checked="" type="checkbox"/>	<input type="checkbox"/>
2	Status bar	<input checked="" type="checkbox"/>	<input type="checkbox"/>
3	Navigation button	<input checked="" type="checkbox"/>	<input type="checkbox"/>
4	Smart switch with multiple functions	<input checked="" type="checkbox"/>	<input type="checkbox"/>
5	USB interface	<input checked="" type="checkbox"/>	<input type="checkbox"/>

รายละเอียดการตรวจสอบ

ขั้นตอนการบริการ

ตรวจสอบระบบไฟฟ้า (Electrical Test)

- ความต้านทานทางไฟฟ้าของเครื่องกับกราวด์
- กระแสไฟฟ้าที่ใช้งาน

ตรวจสอบสภาพเครื่อง (Optical Test)

- Main cable
- Electric wiring
- Pumps
- Distribution Head
- Condensor
- Steam generator
- Tubing
- Viton cone

ตรวจสอบ Function การทำงาน (The Function Test)

- ระบบสร้างและควบคุมความดันของ Steam
- ระบบการเติมน้ำเข้า Sample Tube
- ระบบการเติม Na OH
- ระบบการเติม H₃BO₃

รายงานผลการให้บริการ

1. TECHNICAL DATA

	Pass	Fail	N/A	Remark
Main Supply 220 volt + 10% 50 Hz with ground	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Norminal current	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>8a.....

1.1 COOLING WATER BATH

	Pass	Fail	N/A	Remark
Temperature 15-20 °C	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Cooling Water Outlet	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Control Temperature	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>

1.2 OPTICAL TESTYAP300

	Pass	Fail	N/A	Remark
Screw cap GL14	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Screw cap GL18	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Screw cap GL32	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Distillation Head	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Condensor	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Viton Cone	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Ventilation Valve BV	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Micro Switch Sample	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Agitator motor for propeller	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>

2. SYSTEM COOLING WATER INLET

	Pass	Fail	N/A	Remark
Cooling Water Inlet	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Cooling Water Outlet	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Flow control valve	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>

3.SYSTEM CONTROL

	Pass	Fail	N/A	Remark
Display	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Program	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Adding NaOH	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Adding H2O	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Adding H3BO3	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>
Suction Sample	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Suction Reciver	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>

4.SYSTEM DISTILLATION

	Pass	Fail	N/A	Remark
Boiler	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Level Sensor	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Novopren	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Solenoid Valve Shut-Off	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Solenoid Valve Steam	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Solenoid Valve soft steam	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Ventilation Valve Premount	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Excess Pressure Detector	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Heating Element	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>

ข้อมูลสนับสนุนด้านเทคนิค (General Technical Support)

การบำรุงรักษาทั่วไป (Basic maintenance)

Cleaning program

Glass parts and tubes must be rinsed daily before starting analysis in order to prevent clogging by crystallising chemicals.

The following settings are recommended for this:

parameters	Value
H ₂ O addition	150 ml
NaOH addition	0 ml
Distillation time	7 min
Steam power	100 %
Reaction time	0 s
Suction sample	30 s

➤ Insert a digestion tube (without sample) and start the program.

➤ All liquid carrying parts are cleaned. In the case of strong soiling, approx. 10 ml of sulphuric acid can also be added to the digestion tube.

General error message

Fault description	Cause	Remedy
'Cooling water flow volume too low'	Cooling water pressure under 1 bar	<ul style="list-style-type: none"> ■ Open water tap. ■ Check coolant pressure. ■ Check coolant tube. <p>Program continues automatically once error has been fixed.</p>
'Sample tube missing'	Sample tube missing.	<ul style="list-style-type: none"> ■ Insert sample tube. <p>Continue program or restart.</p>
'Distillation room protective door open'	Protection door not closed	<ul style="list-style-type: none"> ■ Close protection door. <p>Program continues automatically once error has been fixed.</p>
'Reagent storage/waste'	One or more storage tanks are empty	<ul style="list-style-type: none"> ■ Fill storage tank. ■ Check correct seating of the universal sensors. <p>The running program can be continued after rectification of the error.</p>
	The sample waste tank is full.	<ul style="list-style-type: none"> ■ Empty sample waste tank. ■ Check correct seating of the universal sensors. <p>The running program can be continued after rectification of the error.</p>

Analytical errors

Fault description	Cause	Remedy
Analysis results too high	The chemicals used are contaminated with nitrogen compounds.	<ul style="list-style-type: none"> ■ Detailed checking of the chemicals. ■ Determination of a blank value. ■ Replace the chemicals if necessary.
	Violent reaction in the digestion tube, sodium hydroxide drops get into the receiver.	<ul style="list-style-type: none"> ■ Increase of the water addition amount.
	Glass bridge of the condenser is broken or worn out, sodium hydroxide drops get into the receiver.	<ul style="list-style-type: none"> ■ Replacement of the glass condenser.
	Glass cleaning agents in the digestion tube.	<ul style="list-style-type: none"> ■ Clean digestion tube in advance with distilled water.
	Entrainment of ammonia from the previous sample.	<ul style="list-style-type: none"> ■ Increase distillation time. ■ Check whether the sample was previously sufficiently alkalisied.
Analysis result too low or no result	Incomplete distillation; distillation time too short.	<ul style="list-style-type: none"> ■ No quantitative expulsion of the ammonia content. ■ The distillation amount should be 100 ml.
	Ammonia escapes at leaking places.	<ul style="list-style-type: none"> ■ Soiled or defective Viton plugs; clean or replace. ■ Check seals (GL screw connections) on the distribution head; replace if necessary. ■ Check valve at the condenser is gummed up; clean or replace. ■ Digestion tube is damaged at the neck extension. ■ Distribution head glass leaks; replace.
	Addition amount of the sodium hydroxide too little; no ammonia development.	<ul style="list-style-type: none"> ■ Check the constant flow rate of the NaOH pump (see Technical Data).
	Too low boric acid amount in the receiver; escaping ammonia is not completely bonded.	<ul style="list-style-type: none"> ■ Increase of the boric acid amount.
	Tube not completely immersed in the acid receiver.	<ul style="list-style-type: none"> ■ Increase of the acid amount.
	Formation of stable ammonia compounds which are not destroyed with sodium hydroxide.	<ul style="list-style-type: none"> ■ This problem only occurs with catalysts containing mercury. Sodium sulphate solution destroys these compounds.

การดูแลบำรุงรักษาเชิงป้องกัน

Preventive Maintenance



บริษัท ดีเคเอสเอช เทคโนโลยี จำกัด

ฝ่ายบริการหลังการขาย

โทร 0 2 639 7000 E-mail: service.tec.th@dksh.com

ฝ่ายขายและการตลาด

โทร 0 2 639 7000 E-Mail : marketing.tec.th@dksh.com

Website : www.dksh.co.th/technology/scientific-thailand

เงื่อนไขการให้บริการ Preventive Maintenance

บริษัทฯ จะส่งวิศวกรผู้ชำนาญ เพื่อให้บริการตามขอบข่ายของการบริการ เฉพาะ ในวันและเวลา ราชการ หากมีความประสงค์ที่จะรับบริการนอกเหนือจากวัน เวลา ราชการ (วันหยุดเสาร์ – อาทิตย์ หรือวันหยุด นักชัตฤกษ์) บริษัทฯ จะคิดค่าบริการเพิ่มเติมตามอัตราที่กฎหมายแรงงานกำหนดไว้

ขอบข่ายการบริการ

- ตรวจสอบสภาพการทำงานต่าง ๆ ของเครื่องมือ
- ทดสอบประสิทธิภาพการทำงานของเครื่องมือ
- รายการผลการตรวจสอบเครื่องมือ

หมายเหตุ

- ราคานี้ไม่รวมถึงค่าบริการซ่อม หรือ เปลี่ยนอะไหล่ที่ชำรุดเสียหาย หรือหมดสภาพการใช้งาน
- ในกรณีที่ผู้รับบริการอยู่นอกเขตพื้นที่ให้บริการ บริษัทฯ จำเป็นต้องคิดค่าใช้จ่ายเพิ่มเติม ได้แก่ ค่าเดินทาง เป็นต้น
- บริษัท ฯ ขอสงวนสิทธิ์ในการเปลี่ยนแปลงราคา โดยไม่แจ้งให้ทราบล่วงหน้า

ช่องทางการติดต่อ



DKSH Technology Limited (บริษัท ดีเคเอสเอช เทคโนโลยี จำกัด)

เลขที่ 2533 ถนนสุขุมวิท แขวงบางจาก เขตพระโขนง กรุงเทพฯ 10260

เลขประจำตัวผู้เสียภาษี 010-555-001-4547 (สำนักงานใหญ่)



Call center 0 2 639 7000



DKSH Scientific



www.dksh.com/scientific-thailand



marketing.tec.th@dksh.com



@dkshscientific

Preventive Maintenance Contract

จำนวนในการทำสัญญาบริการ ...1... ครั้ง ต่อปี
ครั้งที่ 1 วันที่ 27/03/2024.....

รายละเอียดผู้รับบริการ

หน่วยงาน	บริษัท เทสต์ เทคโนโลยี จำกัด		
ที่อยู่	30,32 ซอยพระรามที่ 2 ซอย 63 ถนนพระรามที่ 2 แขวงสามยุค เขตบางขุนเทียน กรุงเทพมหานคร 10150		
โทรศัพท์	0-2893-4211-7	แฟกซ์	0-2893-4218

ผู้ติดต่อ

ชื่อ - นามสกุล	คุณกรรณก ขุนพิทักษ์				
ตำแหน่ง	หัวหน้าส่วน				
โทรศัพท์	087 398 9274	เบอร์ต่อ	-	แฟกซ์	-
E-mail	lab_center@testtech.co.th				

รายละเอียดผู้ให้บริการ

บริษัท ดีเคเอสเอช เทคโนโลยี จำกัด (ฝ่ายบริการหลังการขาย) (สำนักงานใหญ่)


เลขที่ 2533 ถนนสุขุมวิท แขวงบางจาก เขตพระโขนง กรุงเทพฯ 10260

โทรศัพท์ 0 2 693 7000 Email: sudarat.sk@dksh.com

เจ้าหน้าที่ประสานงาน : คุณสุภารัตน์ ศิริรัตน์ โทรศัพท์ 090 678 6925

เจ้าหน้าที่ผู้ให้บริการ	นายจิรายุส สเลอาด		
ตำแหน่ง	Specialist, Technical Service.		
โทรศัพท์	0938138736	แฟกซ์	-
E-mail	Jirayut.js@dksh.com		

ลงนามผู้รับบริการ	
ตัวบรรจง	(กรรณก ขุนพิทักษ์)
ตำแหน่ง	หัวหน้าส่วนทดสอบน้ำเสีย 2
วันที่ / ประทับตราบริษัท	27/03/2024


ลงนามผู้ให้บริการ	
ตัวบรรจง	(นาย จิรายุส สเลอาด)
ตำแหน่ง	Specialist, Technical Service.
วันที่ / ประทับตราบริษัท	27/03/2024

JOB No: LSPR2402246.....MODEL: Vap30.....S/N: GER003718

Part 1: Operational Qualification (OQ)


ตรวจสอบสภาพเครื่อง

FRONT

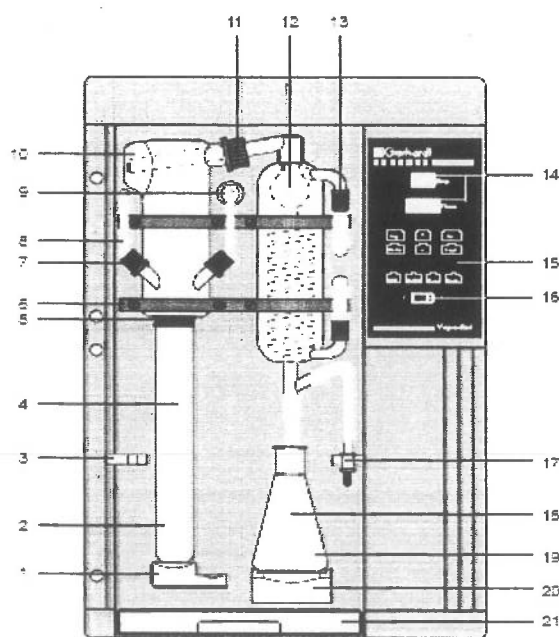

	Pass	Fail	N/A	Remark
1.Quick clamping device with wedge	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
2. Kjeldatherm digestion tube	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
3. Holder for steam inlet tubing	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
4. PTFP-Inlet tubing, steam	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
5. Viton-cone	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
6. Clamping for glassware	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
7. Screw cap GL18 with silicone seal	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
8. PTFP-Inlet tubing, NaOH	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
9. PP-Distributor with PP-threaded joint	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
10. Distribution head, glass	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
11. Screw cap GL32 with silicone seal	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
12. Distillation condenser	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
13. Screw cap GL14 with plastic screw connection	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
14. Display	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
15. Keyboard, chemical-resistant	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
16. Main switch, green	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
17. Ventilation valve	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
18. Distillate outlet tubing	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
19. Erlenmeyer flask	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
20. Platform	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
21. Drip tray	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>

REAR

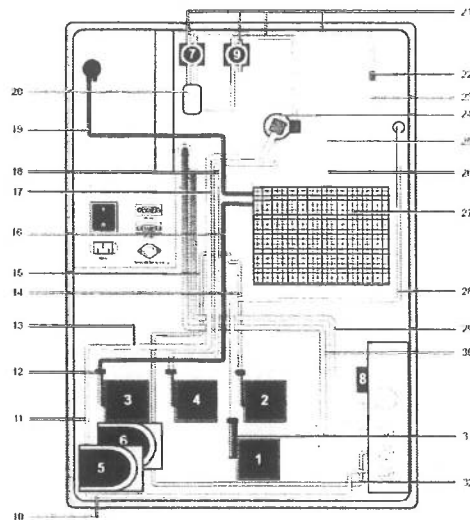

	Pass	Fail	N/A	Remark
1. Diaphragm pump NaOH	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
2. Diaphragm pump H ₃ BO ₃	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	vap 40 only
3. Diaphragm pump H ₂ O for steam generator	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
4. Diaphragm pump H ₂ O for sample	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	vap 30,40 only
5. Peristaltic pump for suction sample	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	vap 30,40 only
6. Peristaltic pump for suction receiver	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	option
7. Pinch-solenoid valve, steam	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
8. Magnetic valve with pressure control	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
9. Pinch-solenoid valve, shut-off	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
10. Verprene-tubing 4x8 mm.	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
11. Verprene-tubing 4x8 mm.	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	vap 30,40 only
12. Non-return valve for diaphragm pumps	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
13. Tubing reduction PP 51x10x5 mm.	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	vap 30,40 only
14. Silicone tubing 4x7 mm.	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	vap 40 only
15. Silicone tubing 4x7 mm.	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	option
16. Silicone -tubing 4x7 mm.	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
17. Verprene-tubing 8x12 mm.	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	vap 30,40 only
18. Verprene tubing 4x7 mm.	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	vap 30,40 only
19. Silicone tubing 4x7 mm.	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
20. Ventilation glass	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
21. Novoprene-tubing 4.8x8 mm.	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
22. Tubing reduction	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
23. Silicone tubing 6x10 mm.	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
24. PP-distributor with PP-thread	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
25. SKT-valve (built in with brass fitting)	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
26. Silicone tubing 8x16x80 mm.	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
27. Steam generator	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
28. PTFE-inlet tubing NaOH	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
29. Silicone tubing 8x16 for cooling water inlet	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
30. Silicone tubing 8x16 for cooling water outlet	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
31. Viton-tubing 6x12*50 mm.	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
32. Silicone tubing 4x7 mm.	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	option

2 รายละเอียดการตรวจสอบ

2.1 ขั้นตอนการบริการ

ตรวจสอบระบบไฟฟ้า (Electrical Test)

- ความต้านทานทางไฟฟ้าของเครื่องกับกราวด์
- กระแสไฟฟ้าที่ใช้งาน

ตรวจสอบสภาพเครื่อง (Optical Test)

- Main cable
- Electric wiring
- Pumps
- Distribution Head
- Condensor
- Steam generator
- Tubing
- Viton cone

ตรวจสอบ Function การทำงาน (The Function Test)

- ระบบสร้างและควบคุมความดันของ Steam
- ระบบการเติมน้ำเข้า Sample Tube
- ระบบการเติม Na OH
- ระบบการ Suction ตั้ง Sample Tube และ Receiver

2.2 รายงานผลการให้บริการ

1. TECHNICAL DATA

	Pass	Fail	N/A	Remark
Main Supply 220 volt + 10% 50 Hz with ground	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Normal current	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>6A....

1.1 COOLING WATER BATH

	Pass	Fail	N/A	Remark
Temperature 15-20 °C	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Cooling Water Outlet	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Control Temperature	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>

1.2 OPTICAL TEST VAP30....

	Pass	Fail	N/A	Remark
Screw cap GL14	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Screw cap GL18	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Screw cap GL32	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Distillation Head	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Condensor	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Viton Cone	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Ventilation Valve	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Micro Switch Sample	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>

2. SYSTEM COOLING WATER INLET

	Pass	Fail	N/A	Remark
Cooling Water Inlet	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Cooling Water Outlet	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Magnetic valve	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>

3.SYSTEM CONTROL

	Pass	Fail	N/A	Remark
Key Board	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Display	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Program	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Adding H ₂ O	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	vap 30,40 only
Adding NaOH	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Adding H ₃ BO ₃	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	vap 40 only
Suction Sample	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	vap 30,40 only

4.SYSTEM DISTILLATION

	Pass	Fail	N/A	Remark
Boiler	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Level Sensor	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Novprene-Tubing	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Solenoid Valve Shut-Off	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Solenoid Valve Steam	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Excess Pressure Detector	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Ventilation Valve	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Heater	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>

5. PUMP

	Pass	Fail	N/A	Remark
Pump H ₂ O Steam	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
- Non-Return Valve	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Pump H ₂ O Sample	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
- Non-Return Valve	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Pump NaOH	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
- Non-Ruturn Valve	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Pump H ₃ BO ₃	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>
- Non-Ruturn Valve	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>
Pump Suction	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>

6. The Following Program Run :

	Pass	Fail	N/A	Remark
Addition H ₂ O 0-99 sec.	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Addition NaOH 0-99 sec.	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Addition H ₃ BO ₃ 0-99 sec.	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>
Reaction Time 0-99 min.	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Distillation Time 0-99 min	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Steam Capacity 30%-100%	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Suction Time 0-99 sec.	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
The Instrument is in perfect technical shape	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>

Remark :

.....

.....

Part 3: ข้อมูลสนับสนุนด้านเทคนิค (General Technical Support)

3.1 การบำรุงรักษาทั่วไป (Basic maintenance)

Cleaning

Glass parts and suction pump should be cleaned before long periods of non-usage (i.e. holidays). This way blockages caused by crystalline deposits are avoided.

The following program should be run:

Addition H_3BO_3	0	s
Addition H_2O :	13	s
Addition NaOH :	0	s
Reaction time:	0	s
Distillation time:	7	min.
Steam capacity:	100	%
Suction time:	20	s

Place an empty digestion tube and an Erlenmeyer flask into position, and start the program.

In case of extreme deposits in the glassware you can clean the system by putting about 10 ml of sulphuric acid into the digestion tube.

3.1 Error Code

The micro-processor continually surveys all the functions of the distillation system. As soon as an error arises it is shown on the display and accompanied by an acoustic signal.

Error message	Measures
No tap water	Check cooling water inlet for blockages. Ensure the tap is turned on → Enter
No sample tube	Insert tube → Enter
Check chemicals	Check set of tanks → Enter
Low water Press Enter	Check the water inlet distilled H ₂ O → Enter
↓ Filling Steam generator	This message disappears as soon as steam generator is filled

After the above mentioned errors are corrected, the following message is displayed.

Error message	Measures
Stop Prog.No. x continue=Enter	Enter = continue of interrupted program Reset = Standby-mode

Other error messages

Error message	Measures
Wait for steam	Message disappears as soon as stand-by is reached
Add sol. > 1mln Continue=Enter	Check programming Enter=continue of interrupted program Reset=Standby-mode
Program undefined	Check programming → Reset
Excess steam pressure	Switch the system off and call service
Sensor error	Switch the system off and call service



CERTIFICATE No : 24T8913
REFERENCE No : 74483-3


PAGE : 1 OF 2

Certificate of Calibration

EQUIPMENT : WATER BATH
MANUFACTURER : N/A
MODEL : SUP IV
SERIAL No : N/A
ID No : EQL-056
CONDITION AS RECEIVED : USED ITEM
SUBMITTED BY : TEST TECH CO., LTD.
30,32 RAMA II SOI 63, RAMA II RD., SAMAEDAM,
BANGKHUNTHIAN, BANGKOK 10150

CALIBRATED BY : PRASERT P.

CALIBRATION DATE : 05-Sep-24

APPROVED BY : 
PONGSAK J.

ISSUED DATE : 09-Sep-24

RECEIVED DATE : 05-Sep-24





QUALITY CALIBRATION CO., LTD.

235 Petchkasem 63/2 Road, Laksong, Bangkai, Bangkok 10160

Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

www.qcalibration.com

CERTIFICATE No : 24T8913

PAGE : 2 OF 2

Calibration Report

EQUIPMENT : WATER BATH
MANUFACTURER : N/A
ID NUMBER : EQL-056
RECEIVED DATE : 05-Sep-24
AMBIENT TEMPERATURE : 24 °C ± 1 °C
MODEL : SUP IV
SERIAL NUMBER : N/A
CALIBRATION DATE : 05-Sep-24
RELATIVE HUMIDITY : 50 %RH ± 10 % RH

CONDITION OF THIS RESULTS OF CALIBRATION


1. THIS INSTRUMENT WAS CALIBRATED ACCORDING TO ASTM E715-80 (REAPPROVED 2001) BY COMPARISON WITH CALIBRATED RTD. THE PROBES WERE PLACED ON FIVE POINTS AND LOCATED ONE PROBE IN EACH OF THE FOUR CORNERS OF THE BATH AND PLACED THE FIFTH RTD WITHIN 2.5 cm. OF THE GEOMETRIC CENTER OF THE WATER VOLUME (REFERENCE LOCATION) UNDER NO LOAD CONDITION.

2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) DATA LOGGER WITH RTD	2625A	6603614	24T6473	01-Jul-25

3. THE CERTIFICATE IS VALID FOR THE ITEM CALIBRATED AS SHOWN ON THE DATE AND PLACE OF CALIBRATION ONLY.
4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.
5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-
- NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH QUALITY CALIBRATION CO., LTD.

RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

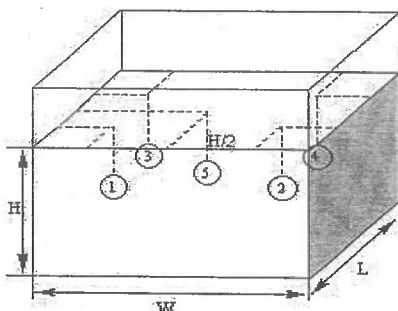

PROBE INSTALLATION
POSITION IN THE BATH

GENERAL INFORMATION

Overall Variation of Ambient Temperature around the Bath (°C) : 0.3
Overall Variation of Line Voltage (V) : 3
Instrument Condition : Normal
Bath Inner Size (W*L*H) : 59*35*20 cm

BATH PERFORMANCE

Calibrate Point (°C)	Average All Position (°C)	Temperature Stability (±°C)	Radius Uniformity (°C)	Axial Uniformity (°C)	Overall Variation (°C)
83.0	82.95	0.17	0.06	0.01	0.41

TEMPERATURE MEASUREMENT ACCURACY TEST

Controller Temp (°C)	Indicating Temp (°C)	Measured Temperature (°C) at Spread Locations					Uncertainty (± °C)
		#1	#2	#3	#4	Ref. 5	
83.0	83.0	82.92	82.96	82.96	82.97	82.93	0.24

NOTE 1 : THE UNCERTAINTY OF MEASUREMENT EXCLUDED TEMPERATURE UNIFORMITY OF THE BATH.

NOTE 2 : THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA.

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR k=2, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT



F-G010 REV : 03



QUALITY CALIBRATION CO.,LTD.

235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160

Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

www.qcalibration.com



CERTIFICATE No : 24T6582

REFERENCE No : 73767-1

PAGE : 1 OF 2

Certificate of Calibration

EQUIPMENT : WATER BATH

MANUFACTURER : MEMMERT

MODEL : WPE 45

SERIAL No : L711.0024

ID No : EQL-147

CONDITION AS RECEIVED : USED ITEM

SUBMITTED BY : TEST TECH CO., LTD.
30,32 RAMA II SOI 63, RAMA II RD., SAMAEDAM,
BANGKHUNTHIAN, BANGKOK 10150

CALIBRATED BY : CHAICHARN CH.

CALIBRATION DATE : 01-Jul-24

APPROVED BY : 
PONGSAK J.

ISSUED DATE : 02-Jul-24

RECEIVED DATE : 01-Jul-24



QUALITY CALIBRATION CO.,LTD.

235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160

Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

www.qcalibration.com

CERTIFICATE No : 24T6582

PAGE : 2 OF 2

Calibration Report

EQUIPMENT : WATER BATH
MANUFACTURER : MEMMERT
ID NUMBER : EQL-147
RECEIVED DATE : 01-Jul-24
AMBIENT TEMPERATURE : 24 °C ± 1 °C
MODEL : WPE 45
SERIAL NUMBER : L711.0024
CALIBRATION DATE : 01-Jul-24
RELATIVE HUMIDITY : 51 %RH ± 10 % RH

CONDITION OF THIS RESULTS OF CALIBRATION


1. THIS INSTRUMENT WAS CALIBRATED ACCORDING TO ASTM E715-80 (REAPPROVED 2001) BY COMPARISON WITH CALIBRATED RTD. THE PROBES WERE PLACED ON FIVE POINTS AND LOCATED ONE PROBE IN EACH OF THE FOUR CORNERS OF THE BATH AND PLACED THE FIFTH RTD WITHIN 2.5 cm. OF THE GEOMETRIC CENTER OF THE WATER VOLUME (REFERENCE LOCATION) UNDER NO LOAD CONDITION.

2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) DATA LOGGER WITH RTD	2625A	6603614	23T6642	19-Jul-24

3. THE CERTIFICATE IS VALID FOR THE ITEM CALIBRATED AS SHOWN ON THE DATE AND PLACE OF CALIBRATION ONLY.
4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.
5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-
- NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH QUALITY CALIBRATION CO.,LTD.

RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

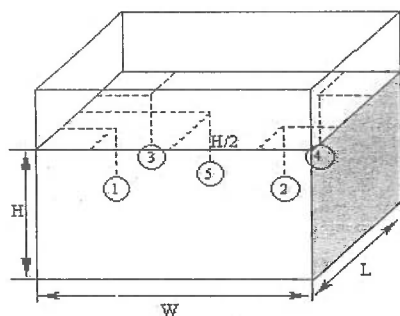

PROBE INSTALLATION
POSITION IN THE BATH

GENERAL INFORMATION

Overall Variation of Ambient Temperature around the Bath (°C) : 1.1
Overall Variation of Line Voltage (V) : 4
Instrument Condition : Normal
Bath Inner Size (W*L*H) : 59*35*22 cm

BATH PERFORMANCE

Calibrate Point (°C)	Average All Position Temp. (±°C)	Temperature Stability (±°C)	Radius Uniformity (°C)	Axial Uniformity (°C)	Overall Variation (°C)
41.5	41.50	0.05	0.04	0.02	0.12
44.5	44.48	0.03	0.03	0.03	0.08

TEMPERATURE MEASUREMENT ACCURACY TEST

Controller Temp (°C)	Indicating Temp (°C)	Measured Temperature (°C) at Spread Locations					Uncertainty (± °C)
		#1	#2	#3	#4	Ref. 5	
41.5	41.5	41.51	41.47	41.51	41.48	41.50	0.14
44.5	44.5	44.47	44.47	44.49	44.47	44.49	0.14

NOTE 1 : THE UNCERTAINTY OF MEASUREMENT EXCLUDED TEMPERATURE UNIFORMITY OF THE BATH.

NOTE 2 : THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA.

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR k=2, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT

F-G010 REV : 03

ภาคผนวก ฉ

หนังสืออนุญาตขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน



ที่ อก ๐๓๑๐(๑)/๗๓๕

กรมโรงงานอุตสาหกรรม
ถนนพระรามที่ ๖ แขวงทุ่งพญาไท
เขตราชเทวี กรุงเทพฯ ๑๐๕๐๐

๒ ๖ มกราคม ๒๕๖๗

เรื่อง ต่ออายุหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน

เรียน กรรมการผู้จัดการ บริษัท เทสต์ เทค จำกัด

อ้างถึง คำขอขึ้นทะเบียน/ต่ออายุ/เปลี่ยนแปลงบุคลากร และชนิดสารมลพิษของห้องปฏิบัติการวิเคราะห์เอกชน
ลงวันที่ ๒๗ ธันวาคม ๒๕๖๖

สิ่งที่ส่งมาด้วย ๑. รายชื่อผู้ควบคุมดูแลห้องปฏิบัติการวิเคราะห์ จำนวน ๑ แผ่น

๒. รายชื่อเจ้าหน้าที่ประจำห้องปฏิบัติการวิเคราะห์ จำนวน ๒ แผ่น

๓. ขอบข่ายสารมลพิษที่ได้รับขึ้นทะเบียนจากกรมโรงงานอุตสาหกรรม จำนวน ๑๔ แผ่น

ตามหนังสือที่อ้างถึง บริษัท เทสต์ เทค จำกัด ขอต่ออายุหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน เลขทะเบียน ว-๒๔๕ สถานที่ตั้งเลขที่ ๓๐,๓๒ ซอยพระรามที่ ๒ ซอย ๖๓ แขวงแสมดำ เขตบางขุนเทียน กรุงเทพมหานครต่อกรมโรงงานอุตสาหกรรม นั้น

กรมโรงงานอุตสาหกรรมพิจารณาแล้ว ให้บริษัท เทสต์ เทค จำกัด ต่ออายุหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน โดยมีองค์ประกอบดังนี้

ก. ผู้ควบคุมดูแลห้องปฏิบัติการวิเคราะห์ จำนวน ๕ ราย ตามสิ่งที่ส่งมาด้วย ๑

ข. เจ้าหน้าที่ประจำห้องปฏิบัติการวิเคราะห์ ๔๔ ราย ตามสิ่งที่ส่งมาด้วย ๒

ค. ขอบข่ายสารมลพิษที่ได้รับขึ้นทะเบียนให้วิเคราะห์ในน้ำเสีย น้ำใต้ดิน สิ่งปฏิกูลหรือวัสดุที่ไม่ใช้แล้ว และดิน ตามสิ่งที่ส่งมาด้วย ๓

หนังสือฉบับนี้จะหมดอายุในวันที่ ๒๘ มกราคม ๒๕๗๐ หากประสงค์จะต่ออายุหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน สามารถยื่นคำขอผ่านระบบอิเล็กทรอนิกส์ได้ที่หน้าเว็บไซต์กรมโรงงานอุตสาหกรรม

จึงเรียนมาเพื่อทราบ

ขอแสดงความนับถือ

(นายประสม ดำรงพงษ์)

ผู้อำนวยการกองวิจัยและเตือนภัยมลพิษโรงงาน
ปฏิบัติราชการแทนอธิบดีกรมโรงงานอุตสาหกรรม

กองวิจัยและเตือนภัยมลพิษโรงงาน

กลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษและทะเบียนห้องปฏิบัติการ

โทร. ๐ ๒๔๓๐ ๖๓๑๒ ต่อ ๒๑๐๓-๕

โทรสาร ๐ ๒๔๓๐ ๖๓๑๒ ต่อ ๒๑๙๙

ไปรษณีย์อิเล็กทรอนิกส์ saraban@diw.mail.go.th



“อุตสาหกรรมก้าวไกล ประเทศไทยก้าวหน้า ร่วมกันพัฒนา อุตสาหกรรมสีเขียว”



เอกสารแนบท้ายหนังสือต่ออายุรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน

บริษัท เทสท์ เทค จำกัด

เลขทะเบียน ว-๒๔๕

ที่ ออก ๐๓๑๐(๑)/ ๗ ๓ ๕

ลงวันที่ ๒๖ มกราคม ๒๕๖๗

ก. ผู้ควบคุมดูแลห้องปฏิบัติการวิเคราะห์ จำนวน ๕ ราย

๑) นางสาวเรวดี ศิริมงคล

ทะเบียนเลขที่ ว-๒๔๕-ค-๐๐๐๑

๒) นางสาวอรษา อยู่บัว

ทะเบียนเลขที่ ว-๒๔๕-ค-๐๐๐๒

๓) นางสาวณัฐวิภา อ่อนจัน

ทะเบียนเลขที่ ว-๒๔๕-ค-๐๐๐๓

๔) นางสาวดวงกมล บุญยิ่ง

ทะเบียนเลขที่ ว-๒๔๕-ค-๐๐๐๔

๕) นางสาวจิตรา ลิ้มสืบพงษ์

ทะเบียนเลขที่ ว-๒๔๕-ค-๐๐๐๕

3mml

เอกสารแนบท้ายหนังสือต่ออายุรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน

บริษัท เทสท์ เทค จำกัด

เลขทะเบียน ว-๒๔๕

ที่ อก ๐๓๑๐(๑)

๗ ๓ ๕

ลงวันที่ ๒๖

มกราคม ๒๕๖๗

ข. เจ้าหน้าที่ประจำห้องปฏิบัติการวิเคราะห์ จำนวน ๔๔ ราย

๑) นางสาวปรางค์ทิพย์ รักษาสุข	ทะเบียนเลขที่ ว-๒๔๕-จ-๐๐๐๔
๒) นางสาวบุษยา ศรีสว่าง	ทะเบียนเลขที่ ว-๒๔๕-จ-๐๐๐๕
๓) นางสาวมินตรา ทิภูงา	ทะเบียนเลขที่ ว-๒๔๕-จ-๐๐๐๗
๔) นายเฉลิมชัย เจริญยิ่ง	ทะเบียนเลขที่ ว-๒๔๕-จ-๐๐๐๘
๕) นายอภิสิทธิ์ คุณมาศ	ทะเบียนเลขที่ ว-๒๔๕-จ-๐๐๐๙
๖) นายชาญวิทย์ อุทัยเลี้ยง	ทะเบียนเลขที่ ว-๒๔๕-จ-๐๐๑๐
๗) นางสาวบุญสิตา พรหมณีนุช	ทะเบียนเลขที่ ว-๒๔๕-จ-๐๐๑๑
๘) นางสาวณัฐนิชา ทองลอย	ทะเบียนเลขที่ ว-๒๔๕-จ-๐๐๑๒
๙) นางสาวฐิติพร เชื้ออรพ	ทะเบียนเลขที่ ว-๒๔๕-จ-๐๐๑๓
๑๐) นางสาวกนกพร มั่นนิยม	ทะเบียนเลขที่ ว-๒๔๕-จ-๐๐๑๔
๑๑) นางสาวนันทิภา สิมพรัักษ์	ทะเบียนเลขที่ ว-๒๔๕-จ-๐๐๑๕
๑๒) นางสาวเบญจมาศ เชื้อหงษ์	ทะเบียนเลขที่ ว-๒๔๕-จ-๐๐๑๖
๑๓) นางสาวสุกษิณ ดวงอินทร์	ทะเบียนเลขที่ ว-๒๔๕-จ-๐๐๑๗
๑๔) นางสาวนุสรินทร์ สุคนธ์ภักดี	ทะเบียนเลขที่ ว-๒๔๕-จ-๐๐๑๘
๑๕) นางสาวชรินทร์ทิพย์ สุขประทุมเนตร	ทะเบียนเลขที่ ว-๒๔๕-จ-๐๐๑๙
๑๖) นางสาวพลอยรุ่ง สุท่ามา	ทะเบียนเลขที่ ว-๒๔๕-จ-๐๐๒๐
๑๗) นางสาวธิตยา ดีมาก	ทะเบียนเลขที่ ว-๒๔๕-จ-๐๐๒๑
๑๘) นางสาวรัชนิกา ลือเฟื่อง	ทะเบียนเลขที่ ว-๒๔๕-จ-๐๐๒๒
๑๙) นางสาวศิริินดา คำดี	ทะเบียนเลขที่ ว-๒๔๕-จ-๐๐๒๓
๒๐) นางสาวลลิตา เสนานุช	ทะเบียนเลขที่ ว-๒๔๕-จ-๐๐๒๔
๒๑) นางสาวโคกษิษฐา ใจดีเฉย	ทะเบียนเลขที่ ว-๒๔๕-จ-๐๐๒๕
๒๒) นายวัฒนา พันธุ์เดช	ทะเบียนเลขที่ ว-๒๔๕-จ-๐๐๒๖
๒๓) นางสาวอ้อยใจ สระจันทร์	ทะเบียนเลขที่ ว-๒๔๕-จ-๐๐๒๗
๒๔) นางสาวมาริสา วิเศษสังข์	ทะเบียนเลขที่ ว-๒๔๕-จ-๐๐๒๘
๒๕) นายณัฐวุฒิ ใจสุภาพ	ทะเบียนเลขที่ ว-๒๔๕-จ-๐๐๒๙
๒๖) นายกิจดิพงษ์ เย็นงาม	ทะเบียนเลขที่ ว-๒๔๕-จ-๐๐๓๐
๒๗) นายไกรทอง สีซอน	ทะเบียนเลขที่ ว-๒๔๕-จ-๐๐๓๑
๒๘) นายสุริยา ชื่นบาน	ทะเบียนเลขที่ ว-๒๔๕-จ-๐๐๓๒
๒๙) นางสาวรัตนรินทร์ ก้องสุรินทร์	ทะเบียนเลขที่ ว-๒๔๕-จ-๐๐๓๓
๓๐) นางสาวนุสรา สุระเวก	ทะเบียนเลขที่ ว-๒๔๕-จ-๐๐๓๔
๓๑) นางสาวนริศรา สอนบุญชู	ทะเบียนเลขที่ ว-๒๔๕-จ-๐๐๓๕
๓๒) นางสาวผ่องอำไพ ยางงาม	ทะเบียนเลขที่ ว-๒๔๕-จ-๐๐๓๖
๓๓) นางสาวนิศาชล อึ้งเกลี้ยง	ทะเบียนเลขที่ ว-๒๔๕-จ-๐๐๓๗
๓๔) นางสาวนริศรา ผงพิลา	ทะเบียนเลขที่ ว-๒๔๕-จ-๐๐๓๘
๓๕) นางสาวคัทลียา หัวหาญ	ทะเบียนเลขที่ ว-๒๔๕-จ-๐๐๓๙

วิมล

๓๖) นางสาวกรรณก ขุนพิทักษ์	ทะเบียนเลขที่ ว-๒๔๕-จ-๐๐๔๐
๓๗) นางสาวดวงหทัย เริ่มวานิชย์	ทะเบียนเลขที่ ว-๒๔๕-จ-๐๐๔๑
๓๘) นางสาวจุไรรัตน์ จงประกอบกิจ	ทะเบียนเลขที่ ว-๒๔๕-จ-๐๐๔๒
๓๙) นายกิตติพิชญ์ ไข่เกตุ	ทะเบียนเลขที่ ว-๒๔๕-จ-๐๐๔๓
๔๐) นางสาวเจนจิรา พลที	ทะเบียนเลขที่ ว-๒๔๕-จ-๐๐๔๔
๔๑) นางสาวชลนิกานต์ สติธรรม	ทะเบียนเลขที่ ว-๒๔๕-จ-๐๐๔๕
๔๒) นางสาวณัฐการณ์ ขวัญศรี	ทะเบียนเลขที่ ว-๒๔๕-จ-๐๐๔๖
๔๓) นายดิษฐ์วัฒน์ นราวิษณุธำรงค์	ทะเบียนเลขที่ ว-๒๔๕-จ-๐๐๔๗
๔๔) นายธนพล สะเอียบคง	ทะเบียนเลขที่ ว-๒๔๕-จ-๐๐๔๘

รพช

เอกสารแนบท้ายหนังสือต่ออายุรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน

บริษัท เทสท์ เทคโนโลยี จำกัด

เลขทะเบียน ว-๒๔๕

ที่ ออก ๐๓๑๐(๑) ๗ ๓ ๕

ลงวันที่ ๒๖ มกราคม ๒๕๖๗

ค. ขอบข่ายสารมลพิษที่ได้รับขึ้นทะเบียนจากกรมโรงงานอุตสาหกรรม จำนวน ๑๓๘ รายการ

น้ำเสีย จำนวน 45 รายการ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
1	Aldrin	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[3]
2	Arsenic	1) Digestion, Hydride Generation/Atomic Absorption Spectrometric Method ^[3] 2) Digestion, Inductively Coupled Plasma Method ^[3]
3	Barium	1) Digestion, Direct Nitrous Oxide-Acetylene Flame Method ^[3] 2) Digestion, Inductively Coupled Plasma Method ^[3]
4	α -BHC	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[3]
5	β -BHC	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[3]
6	δ -BHC	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[3]
7	γ -BHC	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[3]
8	Biochemical Oxygen Demand	1) 5-Day BOD Test, Azide Modification Method ^[3] 2) 5-Day BOD Test, Membrane Electrode Method ^[3]
9	Cadmium	1) Digestion, Direct Air-Acetylene Flame Method ^[3] 2) Digestion, Inductively Coupled Plasma Method ^[3]
10	Chemical Oxygen Demand	1) Open Reflux, Titrimetric Method ^[3] 2) Closed Reflux, Colorimetric Method ^[3] 3) Closed Reflux, Titrimetric Method ^[3]
11	Chlordane	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[3]
12	Chromium	1) Digestion, Direct Air-Acetylene Flame Method ^[3] 2) Digestion, Inductively Coupled Plasma Method ^[3]

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
13	Color	ADMI Weighted-Ordinate Spectrophotometric Method ^[3]
14	Copper	1) Digestion, Direct Air-Acetylene Flame Method ^[3] 2) Digestion, Inductively Coupled Plasma Method ^[3]
15	Cyanide	Distillation, Colorimetric Method ^[3]
16	4,4'-DDD	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[3]
17	4,4'-DDE	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[3]
18	4,4'-DDT	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[3]
19	Dieldrin	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[3]
20	Endosulfan I	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[3]
21	Endosulfan II	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[3]
22	Endosulfan Sulfate	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[3]
23	Endrin	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[3]
24	Endrin Aldehyde	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[3]
25	Formaldehyde	Distillation, Colorimetric Method ^[2]
26	Free Chlorine	1) Iodometric Method ^[3] 2) DPD Colorimetric Method ^[3]
27	Heptachlor	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[3]
28	Heptachlor Epoxide	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[3]
29	Hexavalent Chromium	Colorimetric Method ^[3]

สมชาย

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
30	Lead	1) Digestion, Direct Air-Acetylene Flame Method ^[3] 2) Digestion, Inductively Coupled Plasma Method ^[3]
31	Manganese	1) Digestion, Direct Air-Acetylene Flame Method ^[3] 2) Digestion, Inductively Coupled Plasma Method ^[3]
32	Mercury	Digestion, Cold-Vapor Atomic Absorption Spectrometric Method ^[3]
33	Methoxychlor	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[3]
34	Nickel	1) Digestion, Direct Air-Acetylene Flame Method ^[3] 2) Digestion, Inductively Coupled Plasma Method ^[3]
35	Oil & Grease	1) Liquid-Liquid, Partition-Gravimetric Method ^[3] 2) Soxhlet Extraction Method ^[3]
36	pH	Electrometric Method ^[3]
37	Phenols	Distillation, Direct Photometric Method ^[3]
38	Selenium	1) Digestion, Hydride Generation/Atomic Absorption Spectrometric Method ^[3] 2) Digestion, Inductively Coupled Plasma Method ^[3]
39	Sulfide	1) Iodometric Method ^[3] 2) Methylene blue Method ^[3]
40	Temperature	Laboratory and Field Methods ^[3]
41	Total Dissolved Solids	Dried at 180 °C ^[3]
42	Total Kjeldahl Nitrogen	Macro-Kjeldahl Method ^[3]
43	Total Suspended Solids	Dried from 103 to 105 °C ^[3]
44	Trivalent Chromium	1) Digestion, Direct Air-Acetylene Flame Method; Colorimetric Method; Calculation ^[3] 2) Digestion, Inductively Coupled Plasma Method; Colorimetric Method; Calculation ^[3]
45	Zinc	1) Digestion, Direct Air-Acetylene Flame Method ^[3] 2) Digestion, Inductively Coupled Plasma Method ^[3]

น้ำใต้ดิน จำนวน 56 รายการ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
1	Aldrin	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[3]
2	Antimony	Digestion, Inductively Coupled Plasma Method ^[3]
3	Arsenic	1) Digestion, Hydride Generation/Atomic Absorption Spectrometric Method ^[3] 2) Digestion, Inductively Coupled Plasma Method ^[3]
4	Barium	1) Digestion, Direct Nitrous Oxide-Acetylene Flame Method ^[3] 2) Digestion, Inductively Coupled Plasma Method ^[3]
5	Benzene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[3]
6	Beryllium	1) Digestion, Direct Nitrous Oxide-Acetylene Flame Method ^[3] 2) Digestion, Inductively Coupled Plasma Method ^[3]
7	Bromodichloromethane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[3]
8	Bromoform	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[3]
9	Cadmium	1) Digestion, Direct Air-Acetylene Flame Method ^[3] 2) Digestion, Inductively Coupled Plasma Method ^[3]
10	Carbon tetrachloride	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[3]
11	Chlordane	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[3]
12	Chloroform	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[3]
13	Chlorodibromomethane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[3]
14	Chromium	1) Digestion, Direct Air-Acetylene Flame Method ^[3] 2) Digestion, Inductively Coupled Plasma Method ^[3]

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
15	Chromium (III)	1) Digestion, Direct Air-Acetylene Flame Method; Colorimetric Method; Calculation ^[3] 2) Digestion, Inductively Coupled Plasma Method; Colorimetric Method; Calculation ^[3] .
16	Chromium (VI)	Colorimetric Method ^[3] .
17	Cyanide	Distillation, Colorimetric Method ^[3]
18	1,1-Dichloroethylene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[3]
19	1,2-Dichloroethane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[3]
20	cis-1,2-Dichloroethylene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[3]
21	trans-1,2-Dichloroethylene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[3]
22	DDD	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[3]
23	DDE	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[3]
24	DDT	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[3]
25	Dieldrin	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[3]
26	Endosulfan	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[3]
27	Endrin	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[3]
28	Ethylbenzene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[3]
29	Heptachlor	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[3]
30	Heptachlor epoxide	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[3]


Small

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
31	Hexachlorobenzene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[3]
32	α -HCH	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[3]
33	β -HCH	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[3]
34	γ -HCH	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[3]
35	Lead	1) Digestion, Direct Air-Acetylene Flame Method ^[3] 2) Digestion, Inductively Coupled Plasma Method ^[3]
36	Manganese	1) Digestion, Direct Air-Acetylene Flame Method ^[3] 2) Digestion, Inductively Coupled Plasma Method ^[3]
37	Mercury	Digestion, Cold-Vapor Atomic Absorption Spectrometric Method ^[3]
38	Methoxychlor	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[3]
39	Methylene chloride	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[3]
40	Nickel	1) Digestion, Direct Air-Acetylene Flame Method ^[3] 2) Digestion, Inductively Coupled Plasma Method ^[3]
41	pH	Electrometric Method ^[3]
42	Phenol	Distillation, Direct Photometric Method ^[3]
43	Selenium	1) Digestion, Hydride Generation/Atomic Absorption Spectrometric Method ^[3] 2) Digestion, Inductively Coupled Plasma Method ^[3]
44	Silver	1) Digestion, Direct Air-Acetylene Flame Method ^[3] 2) Digestion, Inductively Coupled Plasma Method ^[3]
45	Styrene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[3]
46	Tetrachloroethylene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[3]

Small

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
47	Toluene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[3]
48	1,1,1-Trichloroethane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[3]
49	1,1,2-Trichloroethane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[3]
50	Trichloroethylene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[3]
51	Vanadium	1) Digestion, Direct Nitrous Oxide-Acetylene Flame Method ^[3] 2) Digestion, Inductively Coupled Plasma Method ^[3]
52	Vinyl chloride	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[3]
53	m-Xylene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[3]
54	o-Xylene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[3]
55	p-Xylene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[3]
56	Zinc	1) Digestion, Direct Air-Acetylene Flame Method ^[3] 2) Digestion, Inductively Coupled Plasma Method ^[3]

สิ่งปฏิกูลหรือวัสดุที่ไม่ใช้แล้ว จำนวน 20 รายการ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
1	Antimony	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[1,4,7] 2) Waste Extraction, Digestion, Flame Atomic Absorption Spectrometric Method ^[1,4,8] 3) Digestion, Inductively Coupled Plasma Method ^[5,7] 4) Digestion, Flame Atomic Absorption Spectrometric Method ^[5,8] 

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
2	Arsenic	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[1,4,7] 2) Waste Extraction, Digestion, Hydride Generation/Atomic Absorption Spectrometric Method ^[1,4,9] 3) Digestion, Inductively Coupled Plasma Method ^[5,7] 4) Digestion, Hydride Generation/Atomic Absorption Spectrometric Method ^[5,9]
3	Barium	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[1,4,7] 2) Waste Extraction, Digestion, Flame Atomic Absorption Spectrometric Method ^[1,4,8] 3) Digestion, Inductively Coupled Plasma Method ^[5,7] 4) Digestion, Flame Atomic Absorption Spectrometric Method ^[5,8]
4	Beryllium	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[1,4,7] 2) Waste Extraction, Digestion, Flame Atomic Absorption Spectrometric Method ^[1,4,8] 3) Digestion, Inductively Coupled Plasma Method ^[5,7] 4) Digestion, Flame Atomic Absorption Spectrometric Method ^[5,8]
5	Cadmium	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[1,4,7] 2) Waste Extraction, Digestion, Flame Atomic Absorption Spectrometric Method ^[1,4,8] 3) Digestion, Inductively Coupled Plasma Method ^[5,7] 4) Digestion, Flame Atomic Absorption Spectrometric Method ^[5,8]
6	Chromium	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[1,4,7] 2) Waste Extraction, Digestion, Flame Atomic Absorption Spectrometric Method ^[1,4,8]

3m2

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
7	Chromium (III)	3) Digestion, Inductively Coupled Plasma Method ^[5,7] 4) Digestion, Flame Atomic Absorption Spectrometric Method ^[5,8] 1) Waste Extraction, Digestion, Inductively Coupled Plasma Method; Waste Extraction, Colorimetric Method; Calculation Method ^[1,4,7,10] 2) Waste Extraction, Digestion, Flame Atomic Absorption Spectrometric Method; Waste Extraction, Colorimetric Method; Calculation Method ^[1,4,8,10] 3) Digestion, Inductively Coupled Plasma Method; Alkaline Digestion, Colorimetric Method; Calculation Method ^[5,6,7,10] 4) Digestion, Flame Atomic Absorption Spectrometric Method; Alkaline Digestion, Colorimetric Method; Calculation Method ^[5,6,8,10]
8	Chromium (VI)	1) Waste Extraction, Colorimetric Method ^[1,10] 2) Alkaline Digestion, Colorimetric Method ^[6,10]
9	Cobalt	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[1,4,7] 2) Waste Extraction, Digestion, Flame Atomic Absorption Spectrometric Method ^[1,4,8] 3) Digestion, Inductively Coupled Plasma Method ^[5,7] 4) Digestion, Flame Atomic Absorption Spectrometric Method ^[5,8]
10	Copper	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[1,4,7] 2) Waste Extraction, Digestion, Flame Atomic Absorption Spectrometric Method ^[1,4,8] 3) Digestion, Inductively Coupled Plasma Method ^[5,7] 4) Digestion, Flame Atomic Absorption Spectrometric Method ^[5,8]

Small

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
11	Lead	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[1,4,7] 2) Waste Extraction, Digestion, Flame Atomic Absorption Spectrometric Method ^[1,4,8] 3) Digestion, Inductively Coupled Plasma Method ^[5,7] 4) Digestion, Flame Atomic Absorption Spectrometric Method ^[5,8]
12	Mercury	1) Waste Extraction, Digestion, Cold-Vapor Atomic Absorption Spectrometric Method ^[1,11] 2) Digestion, Cold-Vapor Atomic Absorption Spectrometric Method ^[12]
13	Molybdenum	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[1,4,7] 2) Waste Extraction, Digestion, Flame Atomic Absorption Spectrometric Method ^[1,4,8] 3) Digestion, Inductively Coupled Plasma Method ^[5,7] 4) Digestion, Flame Atomic Absorption Spectrometric Method ^[5,8]
14	Nickel	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[1,4,7] 2) Waste Extraction, Digestion, Flame Atomic Absorption Spectrometric Method ^[1,4,8] 3) Digestion, Inductively Coupled Plasma Method ^[5,7] 4) Digestion, Flame Atomic Absorption Spectrometric Method ^[5,8]
15	pH	Electrometric Method ^[17,18]
16	Selenium	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[1,4,7] 2) Waste Extraction, Digestion, Hydride Generation/Atomic Absorption Spectrometric Method ^[1,4,13] 3) Digestion, Inductively Coupled Plasma Method ^[5,7]

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
17	Silver	4) Digestion, Hydride Generation/Atomic Absorption Spectrometric Method ^[5,13] 1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[1,4,7] 2) Waste Extraction, Digestion, Flame Atomic Absorption Spectrometric Method ^[1,4,8] 3) Digestion, Inductively Coupled Plasma Method ^[5,7] 4) Digestion, Flame Atomic Absorption Spectrometric Method ^[5,8]
18	Thallium	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[1,4,7] 2) Waste Extraction, Digestion, Flame Atomic Absorption Spectrometric Method ^[1,4,8] 3) Digestion, Inductively Coupled Plasma Method ^[5,7] 4) Digestion, Flame Atomic Absorption Spectrometric Method ^[5,8]
19	Vanadium	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[1,4,7] 2) Waste Extraction, Digestion, Flame Atomic Absorption Spectrometric Method ^[1,4,8] 3) Digestion, Inductively Coupled Plasma Method ^[5,7] 4) Digestion, Flame Atomic Absorption Spectrometric Method ^[5,8]
20	Zinc	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[1,4,7] 2) Waste Extraction, Digestion, Flame Atomic Absorption Spectrometric Method ^[1,4,8] 3) Digestion, Inductively Coupled Plasma Method ^[5,7] 4) Digestion, Flame Atomic Absorption Spectrometric Method ^[5,8]

สมชาย

ดิน จำนวน 17 รายการ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
1	Antimony	1) Digestion, Inductively Coupled Plasma Method ^[5,7] 2) Digestion, Flame Atomic Absorption Spectrometric Method ^[5,8]
2	Arsenic	1) Digestion, Inductively Coupled Plasma Method ^[5,7] 2) Digestion, Hydride Generation/Atomic Absorption Spectrometric Method ^[5,9]
3	Barium	1) Digestion, Inductively Coupled Plasma Method ^[5,7] 2) Digestion, Flame Atomic Absorption Spectrometric Method ^[5,8]
4	Beryllium	1) Digestion, Inductively Coupled Plasma Method ^[5,7] 2) Digestion, Flame Atomic Absorption Spectrometric Method ^[5,8]
5	Cadmium	1) Digestion, Inductively Coupled Plasma Method ^[5,7] 2) Digestion, Flame Atomic Absorption Spectrometric Method ^[5,8]
6	Chromium	1) Digestion, Inductively Coupled Plasma Method ^[5,7] 2) Digestion, Flame Atomic Absorption Spectrometric Method ^[5,8]
7	Chromium (III)	1) Digestion, Inductively Coupled Plasma Method; Alkaline Digestion, Colorimetric Method; Calculation Method ^[5,6,7,10] 2) Digestion, Flame Atomic Absorption Spectrometric Method; Alkaline Digestion, Colorimetric Method; Calculation Method ^[5,6,8,10]
8	Chromium (VI)	Alkaline Digestion, Colorimetric Method ^[6,10]
9	Cyanide	Extraction, Distillation, Colorimetric Method ^[14,15,16]
10	Lead	1) Digestion, Inductively Coupled Plasma Method ^[5,7] 2) Digestion, Flame Atomic Absorption Spectrometric Method ^[5,8]
11	Manganese	1) Digestion, Inductively Coupled Plasma Method ^[5,7] 2) Digestion, Flame Atomic Absorption Spectrometric Method ^[5,8]

Signature

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
12	Mercury	Digestion, Cold-Vapor Atomic Absorption Spectrometric Method ^[12]
13	Nickel	1) Digestion, Inductively Coupled Plasma Method ^[5,7] 2) Digestion, Flame Atomic Absorption Spectrometric Method ^[5,8]
14	Selenium	1) Digestion, Inductively Coupled Plasma Method ^[5,7] 2) Digestion, Hydride Generation/Atomic Absorption Spectrometric Method ^[5,13]
15	Silver	1) Digestion, Inductively Coupled Plasma Method ^[5,7] 2) Digestion, Flame Atomic Absorption Spectrometric Method ^[5,8]
16	Vanadium	1) Digestion, Inductively Coupled Plasma Method ^[5,7] 2) Digestion, Flame Atomic Absorption Spectrometric Method ^[5,8]
17	Zinc	1) Digestion, Inductively Coupled Plasma Method ^[5,7] 2) Digestion, Flame Atomic Absorption Spectrometric Method ^[5,8]

เอกสารอ้างอิง

- กระทรวงอุตสาหกรรม. ประกาศกระทรวงอุตสาหกรรม, พ.ศ. 2566. เรื่อง การจัดการสิ่งปฏิกูลหรือวัสดุที่ไม่ใช้แล้ว. **ราชกิจจานุเบกษา**. 31 พฤษภาคม 2566. เล่มที่ 140 ตอนพิเศษ 126 ง.
- สมาคมวิศวกรรมสิ่งแวดล้อมแห่งประเทศไทย. **คู่มือวิเคราะห์น้ำเสีย**. พิมพ์ครั้งที่ 4. กรุงเทพฯ: เรือนแก้วการพิมพ์, 2547.
- APHA, AWWA, WEF. **Standard Methods for the Examination of Water and Wastewater**. 24th ed. Washington, DC: APHA, 2023.
- United States Environmental Protection Agency. **Test Methods for Evaluation Solid Waste Physical/Chemical Methods**. SW-846, 2014.
- United States Environmental Protection Agency. **Test Methods for Evaluation Solid Waste Physical/Chemical Methods**. **Acid Digestion of Sediments, Sludges, and Soils**. SW-846 Method 3050B, 2007.
- United States Environmental Protection Agency. **Test Methods for Evaluation Solid Waste Physical/Chemical Methods**. **Alkaline Digestion for Hexavalent Chromium**. SW-846 Method 3060A, 1996.

7. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Inductively Coupled Plasma-Optical Emission Spectrometry. SW-846 Method 6010C**, 2000.

8. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Flame Atomic Absorption Spectrophotometry. SW-846 Method 7000B**, 2007.

9. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Antimony and Arsenic (Atomic Absorption, Borohydride Reduction). SW-846 Method 7062**, 1994.

10. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Chromium, Hexavalent (Colorimetric). SW-846 Method 7196A**, 1992.

11. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Mercury in Liquid Waste (Manual Cold-Vapor Technique). SW-846 Method 7470A**, 1994.

12. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Mercury in Solid or Semisolid Waste (Manual Cold-Vapor Technique). SW-846 Method 7471B**, 2007.

13. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Selenium (Atomic Absorption, Borohydride Reduction). SW-846 Method 7742**, 1994.

14. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Total and Amenable Cyanide: Distillation. SW-846 Method 9010C**, 2004.

15. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Cyanide Extraction Procedure for Solids and Oil. SW-846 Method 9013A**, 1996.

16. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Cyanide in Waters and Extracts Using Titrimetric and Manual Spectrophotometric Procedures. SW-846 Method 9014**, 2014.

17. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **pH Electrometric Measurement. SW-846 Method 9040C**, 2004.

18. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Soil and Waste pH. SW-846 Method 9045D**, 2004.

3กม.1