


ภาคผนวก จ

เอกสารรับรองการสอบเทียบเครื่องมือ

---

รายการใบรับรองสอบเทียบ/ทวนสอบ เครื่องมือหลักประจำห้องปฏิบัติการวิเคราะห์ สำหรับวิเคราะห์คุณภาพสิ่งแวดล้อม

No.	Instrument/Equipment	Parameter	Manufacturer	Model/Serial No.	Calibrator	Certification No.	Date of Calibration	Due date of Calibration*	Remark
เครื่องมือหลักประจำห้องปฏิบัติการวิเคราะห์คุณภาพน้ำ									
1	pH Meter	ความเป็นกรดและด่าง	Mettler-Toledo	Seven Easy S20 / 1230525212	DKSH (Thailand) Ltd.	C07240167	9 Apr 24	8 Apr 25	-
2	pH Meter		HANNA Instruments	HI2020-02 C0051107	National Food Institute, Ministry of Industry, Thailand	2404042-00101	14 Aug 24	14 Aug 25	-
3	Turbidity Meter	ความขุ่น	Oakton	T100IR / 1120501017	Technology Promotion Association (Thailand-Japan)	23CH1148	6 Sep 24	6 Sep 25	-
4	Analytical Balance (Readability 0.01 mg)	ของแข็งแขวนลอย	Mettler-Toledo	XSR205DU / C210685394	National Food Institute, Ministry of Industry, Thailand	2402283-002-01	2 Apr 24	1 Apr 25	-
5	Hot Air Oven		Memmert	UF55 / B216.1666	National Food Institute, Ministry of Industry, Thailand	2400141-001-01	8 Oct 24	8 Oct 25	-
6	Analytical Balance (Readability 0.1 mg)	น้ำมันและไขมัน	Mettler-Toledo	XSR204 / C117635043	Technology Promotion Association (Thailand-Japan)	24MM293	11 May 24	10 May 25	-
7	BOD Incubator	บีโอดี	Arco	UC4-1320 / (UAE.WAO.015/2561)	Technology Promotion Association (Thailand-Japan)	24TM303	10 Feb 24	9 Feb 25	-
8	DO Meter		YSI	5100 / 11B101863	Technology Promotion Association (Thailand-Japan)	24TW39	21 Feb 24	20 Feb 25	-
9	COD Reactor (Heating Block)	ซีโอดี	Hanna	HI839800 / 1147807	Hanna Instruments (Thailand) Ltd.	HIT-2417-0568	25 Apr 24	24 Apr 25	-
10	UV-VIS Spectrophotometer		Agilent Technologies	Cary60 G6860A / MY15410009	DQE Services Co.,Ltd.	SP24-018	7 May 24	6 May 25	-
11	Incubator	แบคทีเรียกลุ่มโคลิฟอร์มทั้งหมด	Memmert	IPP 260 / V615.0187	Technology Promotion Association (Thailand-Japan)	24TM648	1 Apr 24	1 Apr 25	-
12	Water Bath		Memmert	WNE 14 / L416.0606	Technology Promotion Association (Thailand-Japan)	24TM29	10 Feb 24	8 Feb 25	-
13	Auto Clave		ALP	CL-40L / 808763	National Food Institute, Ministry of Industry, Thailand	2402281-00101	2 Apr 24	2 Apr 25	-
14	Analytical Balance		OHAUS	PX623 / C236754745	National Food Institute, Ministry of Industry, Thailand	2402419-001-01	19 Apr 24	19 Apr 25	-



# Certificate of Calibration

**Equipment:** pH METER Certificate No.: C07240167  
**Model:** SevenEasy Issued Date: 9 April 2024  
**Serial No. (or ID.):** 1230525212 (UAE.WAS.003/2553) Job No.: WO-00024208  
**Manufacturer:** METTLER TOLEDO Page: 1 of 3  
**Electrode Serial No.:** 1156883 Model: InLab Solids Brand: METTLER TOLEDO  
**Condition:** In Condition

**Customer:** United Analyst and Engineering Consultant Company Limited  
3 Soi Udomsuk 41 Sukhumvit Road,  
Bangkok, Prakanong, Bangkok 10260 Thailand

**Environment Condition:** Temperature 23 °C  $\pm$  2 °C  
Humidity 50 %RH  $\pm$  15 %RH

**Calibration Place:** Environment Laboratory, DKSH Technology Limited.  
2533 Sukhumvit Road, Bangchak,  
Phrakhanong, Bangkok 10260 Thailand

**Calibration By:** Miss.Orawan Khlaiphloi

**Calibration Date:** 9 April 2024

**The Method used:** In house method, CAL-WI-58, base on ASTM E 70-07

**Traceability:** This certificate is traceable to SI Units, Sample Test is assured through primary measurement method Harned cell, through CPAchem Ltd. (ISO/IEC 17034) Certificate No. 938377, 931985, 931984 And pH Scale traceable to the SI Units maintained by National Institute of Metrology (NIMT), Thailand through Industrial Foundation Electrical and Electronics Institute Certificate No. CA20230350EA

(Miss Orawan Khlaiphloi)

Person in charge

(Mr. Nitinun Srihawan)

Authorized signatory

This certificate is issued the units of measurement according to the International System of Units (SI). It provides traceability of measurement to international or national standard or other recognized national standard laboratories.

The measurement uncertainty stated is the expanded uncertainty which is obtained from the standard uncertainty multiplied by the coverage factor ( $k=2$ ) to provide a level of confidence of approximately 95%. It is determined in accordance with the Guide to Expression of Uncertainty in Measurement (GUM).

These results may be affected by deviations from specified conditions. The results relate only to the items tested, calibrated or sampled. The report shall not be reproduced except in full without approval of DKSH Technology Limited.

## Calibration Results:

### pH Scale

Input	pH Meter Reading			Uncertainty of Measurement (mV)	Coverage Factor (k)
	(mV)	Error (mV)	(pH)		
414.12	414	-0.12	0.00	0.58	2.00
354.96	355	0.04	1.00	0.58	2.00
295.8	296	0.20	2.00	0.58	2.00
236.64	237	0.36	3.00	0.58	2.00
177.48	178	0.52	4.00	0.58	2.00
118.32	118	-0.32	5.00	0.58	2.00
59.16	59	-0.16	6.00	0.58	2.00
0	0	0.00	7.00	0.58	2.00
-59.16	-59	0.16	8.00	0.58	2.00
-118.32	-118	0.32	9.00	0.58	2.00
-177.48	-177	0.48	10.00	0.58	2.00
-236.64	-236	0.64	11.00	0.58	2.00
-295.8	-296	-0.20	12.00	0.58	2.00
-354.96	-355	-0.04	13.00	0.58	2.00
-414.12	-414	0.12	14.00	0.58	2.00



**Practical slope and zero point\***

The three-point calibration using three standard buffer solutions; pH 4.008 , pH 6.985 and pH 9.997

-During calibration, display of pH meter reading; pH 4.00 , pH 7.00 and pH 10.01

The practical slope of the pH electrode; 57.01 (mV/pH), 96.37%


The zero point of the pH electrode; 6.88 (pH)

**Sample Test Results**

Standard Buffer Solution (pH)	Unit Under Calibration (pH)	Difference (pH)	Uncertainty of Measurement (pH)	Coverage Factor (k)
4.008	3.99	-0.018	0.0070	2.00
6.985	7.00	0.015	0.0091	2.00
9.997	10.02	0.023	0.0074	2.00

\* Calibration Marked " Not TISI Accredited " in this Certificate have been included for completeness.

**The End of Certificate**

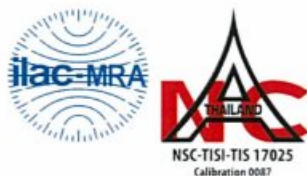

## Certificate of Calibration

<b>Equipment:</b>	Digital Thermometer with Probe	<b>Certificate No.:</b>	C15240373
<b>Model:</b>	SevenEasy pH	<b>Issued Date:</b>	09 April 2024
<b>Serial No.:</b>	1230525212	<b>Job No.:</b>	WO-00024208
<b>Manufacturer:</b>	METTLER TOLEDO	<b>Page:</b>	1 of 2
<b>ID No.:</b>	UAE.WAS.003/2553	<b>Condition:</b>	In Condition

**Customer:** United Analyst and Engineering Consultant Company Limited  
3 Soi Udomsuk 41 Sukhumvit Road,  
Bangkok, Prakanong, Bangkok 10260 Thailand

**Environment Condition:** Temperature: 22 °C ± 3 °C  
Humidity: 50 %RH ± 20 %RH  
Voltage: 220 VAC ± 10 %

**Calibration Place:** Thermo-Hygro Laboratory, DKSH Technology Limited.  
2533 Sukhumvit Road, Bangchak,  
Phrakhanong, Bangkok 10260 Thailand

**Calibration By:** Mr. Nateekarn Mitjit

**Calibration Date:** 09 April 2024

**The Method used:** In house method, CAL-WI-19, by comparison with standard thermometer

**Traceability:** This certificate is traceable to the International System of Unit maintained by Quality Reborn Co.,Ltd. (QR) Certificate No. QR23-1073

(Mr. Nateekarn Mitjit)

Person in charge

(Mr. Pramote Ramrong)

Authorized signatory

This certificate is issued the units of measurement according to the International System of Units (SI). It provides traceability of measurement to international or national standard or other recognized national standard laboratories.

The measurement uncertainty stated is the expanded uncertainty which is obtained from the standard uncertainty multiplied by the coverage factor ( $k=2$ ) to provide a level of confidence of approximately 95%. It is determined in accordance with the Guide to Expression of Uncertainty in Measurement (GUM).

These results may be affected by deviations from specified conditions. The results relate only to the items tested, calibrated or sampled. The report shall not be reproduced except in full without approval of DKSH Technology Limited.

**Reference standard equipment:**

Equipment	Certificate no	Cal. date	Next Cal. date
Digital Thermometer with Probe	QR23-1073	2 May 23	2 May 24

**Calibration Results:****Without Adjustment**

Sensor Type: RTD

Channel: -


Diameter (mm) 4

Length (mm): 135

Immersion (mm): 110

Calibrate Point.(°C)	STD. Reading (°C)	UUC. Reading (°C)	Correction of UUC (°C)	Uncertainty ( $\pm$ °C)
15.0	15.010	15.1	-0.090	0.076
25.0	25.006	25.1	-0.094	0.076
35.0	35.004	35.0	0.004	0.076

**The End of Certificate**

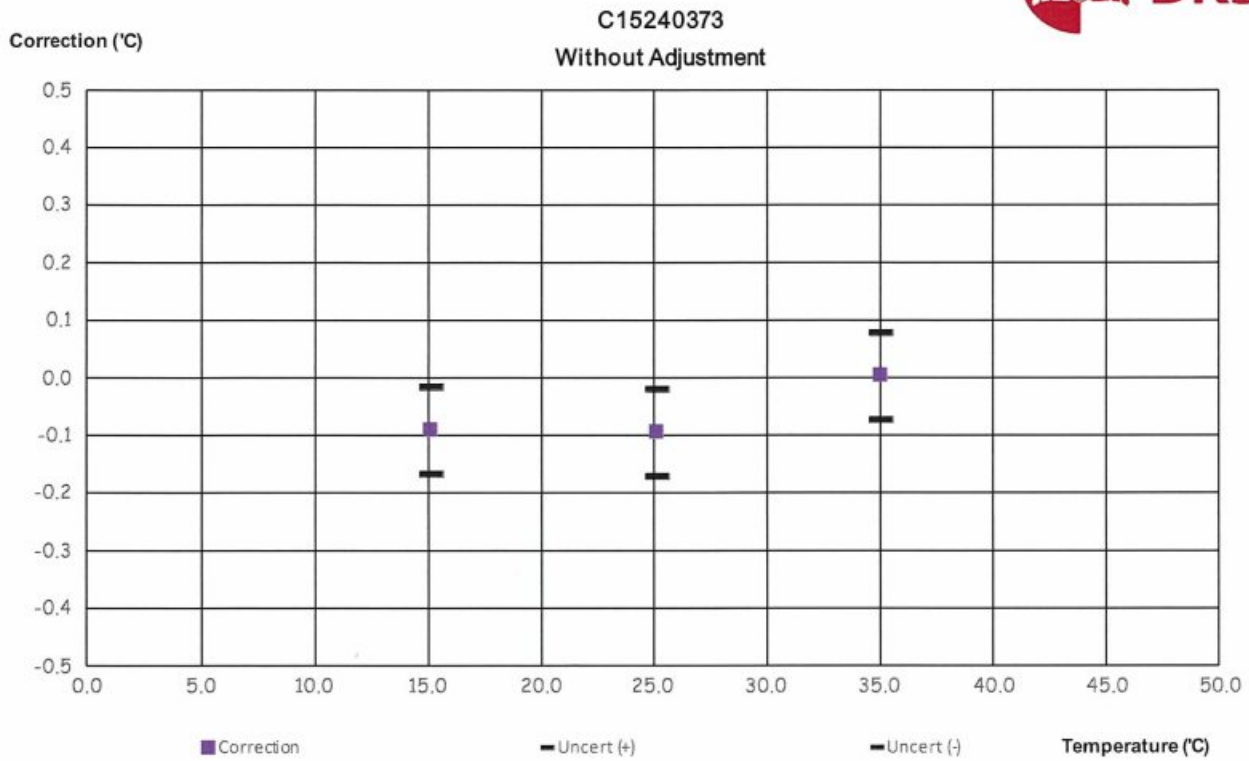


## Calibration Certificate

**Certificate No.:** 2404042-001-01  
**Client name:** UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.  
**Address:** 3 Soi Udomsuk 41, Sukhumvit Road,  
Bangchack, Prakhong, Bangkok 10260

Page 1 of 5

**Equipment:** pH Meter  
**Manufacturer:** HANNA Instruments  
**Model:** HI2020-02  
**Serial No.:** C0051107  
**ID No.:** UAE.WAO.005/2557  
**Order No.:** 2404042  
**Operation No.:** 2404042-001  
**Date of Receipt:** 14 August 2024  
**Date of Calibration:** 21 August 2024

**Calibrated by** Mr.Manas Somsak  
Specialist

**Approved by**   
( Mr.Pheraphat Tuanjit )  
Manager, Division of Calibration Laboratory

**Date of Issue:** 21 August 2024 **Responsible for the Technical Management Team**

The uncertainties are for a confidence probability of approximately 95%.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the National Food Institute.

F-CS-009 Revision: 01 Date: 20-04-65



## Calibration Report

**Certificate No.:** 2404042-001-01

**Equipment:**

pH Meter

**Resolution:** 0.001 pH ; 0.1 mV

**Manufacturer:** HANNA Instruments

**Model:** HI2020-02

**Serial No.:** C0051107

**Type:** Bench top

**ID No.:** UAE.WAO.005/2557

**Date of Calibration:** 21 August 2024

Page 2 of 5

**Location:** Chemical Calibration Laboratory, National Food Institute

**Environment Condition:** **Ambient Temperature:** ( 23.1 ± 1.5 ) °C **Relative Humidity:** ( 55 ± 3 ) %

**Condition of Equipment:** Good Condition

**Condition of this Results of Calibration**

1. Calibration Method W-CC-002 : In house method based on direct measurement by using standard voltage calibrator and certified reference material (CRM)

2. Reference Standards / Certified Reference Material

Instruments	Serial / ID No.	Manufacturer	Certificate No.	Due Date
2.1 DC Voltage Calibrator	2709007	Fluke	24E1752	30 May 2025
2.2 Digital Thermometer	2709007	Fluke	CC 660570-01	30 October 2024
2.3 Thermo-Hygro Meter	NFI.BTH 019/23	testo	QR24-0492	4 March 2025
Certified Reference Material	Lot. No.	Manufacturer	Ref N	Expire Date
2.4 pH buffer 4.008 (Primary pH buffer Solution)	873608	CPAchem	PH216.L5	16 February 2025
2.5 pH buffer 6.865 (Primary pH buffer Solution)	873609	CPAchem	PH217.L5	16 February 2025
2.6 pH buffer 10.01 (Primary pH buffer Solution)	949189	CPAchem	PH220.L5	30 November 2024
2.7 pH buffer 7.00 (Standard pH buffer Solution)	C03109	HACH LANGE GmbH	S11M004	16 October 2025

3. This certification is traceable to The International System of Unit (SI Unit)

3.1 Instruments No.2.1	through	NSC-TISI-TIS 17025 Laboratory Accreditation of Calibration No.0008
3.2 Instruments No.2.2	through	NSC-TISI-TIS 17025 Laboratory Accreditation of Calibration No.0061
3.3 Instruments No.2.3	through	NSC-TISI-TIS 17025 Laboratory Accreditation of Calibration No.0292
3.4 Certified Reference Material No.2.4 to 2.6	traceable to	Primary measurement method- Harned cell using calibrated thermometer, barometer, and nanovoltmeter. The Standard Solution preparation and certified by CPAchem Ltd is accredited to ISO 17034 and ISO/IEC 17025
3.5 Certified Reference Material No.2.7	traceable to	PTB Certificate Nr. PTB-PHOA-563/30504/23 and Certificate Nr. PTB-PHOB-555/30620/22 (PTB: Physikalisch-Technische Bundesanstalt, Braunschweig, Germany)

4. This certificate was certified only for the instrument we calibrated.

5. This result of calibration was found accurate as shown on date and place of calibration only.

F-CS-012 Revision: 01 Date: 20-04-65

## Calibration Report

**Certificate No.:** 2404042-001-01

**Equipment:** pH Meter **Resolution:** 0.001 pH ; 0.1 mV

**Manufacturer:** HANNA Instruments **Model:** HI2020-02

**Serial No.:** C0051107 **Type:** Bench top

**ID No.:** UAE.WAO.005/2557

**Date of Calibration:** 21 August 2024

Page 3 of 5

### Calibration Results:

#### 1. Calibration of pH Meter ( Manual Temperature Compensation at 25 °C )

Nominal pH	DC Voltage Standard ( mV )	Average Indicator Reading		Uncertainty ( ±mV )	Coverage Factor ( k )
		mV	pH		
0	414.122	421.0	-0.001	0.063	2.00
2	295.815	302.7	1.999	0.063	2.00
4	177.463	184.3	4.000	0.063	2.00
6	59.160	66.0	6.000	0.063	2.00
7	0.001	6.8	7.001	0.063	2.00
8	-59.159	-52.3	8.000	0.063	2.00
10	-177.462	-170.6	10.000	0.063	2.00
12	-295.813	-289.0	12.002	0.063	2.00
14	-414.121	-407.3	14.002	0.063	2.00

#### 2. Calibration of pH Meter with Electrode ( Manual Temperature Compensation at 25 °C )

**Equipment:** pH Electrode **Type:** Combined Electrode

**Manufacturer:** HANNA Instruments **Model:** HI11310

**Serial No.:** 539960 **ID.No.:** N/A

**Performance of Electrode system** (Three-Point Calibration at pH 4, 7 and 10)

Certified Value @25 °C (pH)	Average Indicator Reading		Relative Slope (%)	Uncertainty ( ± pH )	Coverage Factor ( k )
	pH	mV			
4.008	4.011	173.4	-	0.0043	2.00
7.001	7.004	-1.6	98.8	0.0073	2.00
9.997	10.011	-175.9	98.0	0.0073	2.00
6.865	6.870	6.4	-	0.0049	2.00



## Calibration Report

**Certificate No.:** 2404042-001-01

**Equipment:** Digital Thermometer with RTD (pH Meter)

**Resolution:** 0.1 °C **Model:** HI2020-02

**Serial No.:** C0051107 **ID No.:** UAE.WAO.005/2557

**Manufacturer:** HANNA Instruments

**Date of Calibration:** 21 August 2024

Page 4 of 5

**Location:** Chemical Calibration Laboratory, National Food Institute

**Environment Condition:**

<b>Ambient Temperature</b>	23 °C	±	1 °C
<b>Relative Humidity</b>	55 %	±	3 %

### Condition of this results of Calibration:

- Calibration Method :
  - In house method: W-TE-025 by comparison with standard thermometer.
  - The Calibration is determined by comparing with a known temperature from a standard resistance thermometer.
  - The temperature scale in use at this laboratory is the International Temperature scale of 1990 ( ITS-90 ).

### 2. Reference Standard Instrument :

Instrument	Model	Serial No.	Certificate No.	Due Date	Through
HANDHELD THERMOMETER	1521	A85997	TE 670101-01	16-Dec-24	NATIONAL FOOD INSTITUTE
Platinum Resistance Thermometer (PRT)	385	509201			

Support Equipment : - Low Temperature Bath (AMETEK RTC-187), Model: RTC-187C , S/N: 670930-00018

- This certificate is traceable to International System of Units (SI Units).
- This certificate was certified only for the instrument we calibrated.
- This result of calibration was found accurate as shown on date and place of calibration only.

6. Condition of Calibrated item : Good

7. Result of Calibration : ☒ Without adjustment ☐ After adjustment

## Calibration Report

**Certificate No.:** 2404042-001-01

**Equipment:** Digital Thermometer with RTD (pH Meter)

Resolution: 0.1 °C      Model: HI2020-02

Serial No.: C0051107      ID No.: UAE.WAO.005/2557

Manufacturer: HANNA Instruments

**Date of Calibration:** 21 August 2024

Page 5 of 5

**Calibration point:** 15.0, 20.0 and 25.0 °C

**Calibration result:**

- The probe was immersed in liquid bath or dry bath to a minimum depth of 120 mm.
- Description of probe, model : HI11310      S/N : 539960
- Dimension of probe : Diameter 12 mm., Length 120 mm.,
- Sheath material : Glass

UUC* Reading (°C)	Standard Temperature (°C)	Correction Value (°C)	Uncertainty ± (°C)
15.0	14.998	0.0	0.099
20.0	19.999	0.0	0.099
25.0	24.999	0.0	0.099

Note

- UUC\* : Unit Under Calibration

The report uncertainty of measurement was based on standard uncertainty multiplied by coverage factor  $k=2$ , providing a level of confidence of approximately 95 %.

----- End -----


F-CS-012 Revision: 01 Date: 20-04-65



## Certificate of Calibration

Cert.No.: 24CH1115

Page.: 1 of 2

Equipment : Turbidity Meter  
Manufacturer : Oakton  
Model : T100IR  
Serial No. : 1120501017  
ID. No. : UAE.WAT.056/2563  
Condition As-Received: Used Item  
Received Date : 05 September 2024  
Calibration Date : 06 September 2024  
Reference : 2409-0177DSC-1  
Submitted by : United Analyst and Engineering Consultant Co.,Ltd.  
3 Soi Udomsuk 41, Sukhumvit Road,  
Bangchak, Phrakhanong, Bangkok 10260  
Ambient Temperature : (25  $\pm$  2.5) °C  
Relative Humidity : (50  $\pm$  20) %  
Calibration Procedure : In - house method : CP-CH11  
Direct measurement by  
using Formazin standard solution  
Calibrated by : Walalak Sirithean  
Approved by :   
Approved Signatory  
( ) Unnopphol Harachai  
( ) Ponpan Paipim  
(✓) Saithip Meangmai  
Issue Date : 9 September 2024

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written  
Approval of the head of Calibration and Testing Equipment Services.

เอกสารไม่ควบคุม





Cert.No. : 24CH1115

Page. : 2 of 2

**Condition of this calibration result**

1. Reference Standard Instruments :

<u>Instruments</u>	<u>Serial No.</u>	<u>ID No.</u>	<u>Certificate No.</u>	<u>Due date</u>
1) Thermo-Hygrograph	1103328	130EC010	24H1372	12 July 2025
2) Electronic Balance	1126143764	140RC004	22MM22	20 Feb 2025

- This Certification is traceable to SI Through Technology Promotion Association (Thailand - Japan)

2. Standard Material : The Formazin suspension has been prepared gravimetric from

<u>Material</u>	<u>Manufacturer</u>	<u>Lot No.</u>	<u>Assay</u>
1) Hexamethylenetetramine	HIMEDIA	0000493947	99.65%
2) Hydrazinium Sulfate	HIMEDIA	0000522014	99.40%

3. This certificate is valid only to the item calibrated on date and place of calibration.

**Calibration result**

Performing five - Formazin suspension standard curve by using 0,20,100,400,800 NTU  
Turbidity Meter Serial Number : 1120501017

Standard Formazine suspension ( NTU )	UUC* Reading ( NTU )	Uncertainty of Measurement ( $\pm$ NTU )	Coverage Factor <i>k</i>
0	0.00	0.0081	2.06
20	20.2	0.39	2.00
100	100	0.75	2.00
400	401	1.5	2.06
800	801	2.1	2.17

**Remark** - UUC\* = Unit Under Calibration  
- NTU = Nephelometric Turbidity Units

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k* , providing a level of confidence of approximately 95 %.

-o0o-

เอกสารไม่ควบคุม

## Calibration Certificate

**Certificate No.:** 2402283-002-01  
**Client name:** UNITED ANALYST AND ENGINEERING CONSULTANT CO., LTD.  
**Address:** 3 SOI UDOMSUK 41, SUKHUMVIT ROAD,  
Bangchack, Prakhnong, Bangkok 10260

Page 1 of 4

**Equipment:** Electronic Balance  
**Manufacturer:** METTLER TOLEDO  
**Model:** XSR205DU  
**Serial No.:** C210685394  
**ID No.:** UAE.WAO.010/2565  
**Order No.:** 2402283  
**Operation No.:** 2402283-002  
**Date of Receipt:** 2 April 2024  
**Date of Calibration:** 2 April 2024

**Calibrated by** Mr.Jerawut Prapawuttipong  
Scientist

**Approved by**

( Mr.Pheraphat Tuanjit )

Manager, Division of Calibration Laboratory

**Date of Issue:** 9 April 2024

Responsible for the Technical Management Team

**The uncertainties are for a confidence probability of approximately 95%**

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the National Food Institute.

F-CS-009 Revision: 01 Date: 20-04-65



# Calibration Report

**Certificate No.:** 2402283-002-01

**Equipment:**

Electronic Balance

**Manufacturer:** METTLER TOLEDO

**Model:** XSR205DU

**Resolution:** 0.00001 g / 0.0001 g

**Serial No.:** C210685394

**ID No.:** UAE.WAO.010/2565

**Capacity:** 220 g

**Date of Calibration:** 2 April 2024

Page 2 of 4

**Environment Condition:** Ambient Temperature: 24.5 ± 0.5 °C Relative Humidity: 47.5 ± 2.5 %

**Place of Calibration:** Laboratory, UNITED ANALYST AND ENGINEERING CONSULTANT CO., LTD.

**Condition of Equipment:** Good Condition

## Condition of This Results of Calibration:

1. Calibration Method: NFI Method W-MA-001 In-House Method based on UKAS Lab 14 : 2019

2. Reference Standards:

Reference Standard	Model	Serial No.	Calibrated By	Certificate No.	Due Date
Standard Weight Class E2	1mg to 200g	B505567572	TCS	M2304053S	8 April 2024

Instrument	Model	Serial No.	Calibrated By	Certificate No.	Due Date
Thermo-Hygro Meter	608-H1	NFI.BTH 016/23	Quality Reborn	QR24-0343	9 February 2025

3. This certification is traceable to SI UNIT

4. This certificate was certified only for the instrument we calibrated.

5. This result of calibration was found accurate as shown on date and place of calibration only.

## Calibration Results:




### 1. Repeatability of Reading:

Nominal Value ( g )	Standard Deviation of Reading ( g )
40	0.0000042
80	0.0000052
100	0.000048
200	0.000048

### 2. Off-Center Error:

A mass of 100 g was placed and moved to various position on pan.

The balance reading obtained is given in the table.



1 ( g )	2 ( g )	3 ( g )	4 ( g )	5 ( g )	6 ( g )	(Maximum Difference) ( g )
100.0000	100.0001	99.9999	99.9999	100.0001	100.0000	0.0001

# Calibration Report

**Certificate No.:** 2402283-002-01

**Equipment:**

Electronic Balance

**Manufacturer:** METTLER TOLEDO

**Model:** XSR205DU

**Resolution:** 0.00001 g / 0.0001 g

**Serial No.:** C210685394

**ID No.:** UAE.WAO.010/2565

**Capacity:** 220 g

**Date of Calibration:** 2 April 2024

Page 3 of 4

**Calibration Results:** (Continued)

**Calibration Range:** 0 - 80 g

**Calibration Adjustment:** Internal Calibration

**3. Departure from Nominal Value:** (Range: 0 - 80 g ; Resolution: 0.00001 g )

Nominal Value ( g )	Standard Value ( g )	Average Reading ( g )	Correction ( g )	Uncertainty ( ± g )	Coverage Factor k
Unload	0.000000	0.00000	0.00000	0.0000086	2.00
0.001	0.001003	0.00101	-0.00001	0.0000089	2.00
0.005	0.005003	0.00500	0.00000	0.0000092	2.00
0.01	0.010003	0.01000	0.00000	0.0000089	2.00
0.05	0.049996	0.05000	0.00000	0.0000096	2.00
0.1	0.100011	0.10000	0.00001	0.000011	2.00
0.5	0.500016	0.50001	0.00001	0.000014	2.00
1	1.000003	1.00002	-0.00002	0.000016	2.00
2	2.000023	2.00001	0.00001	0.000017	2.00
5	5.000017	5.00002	0.00000	0.000020	2.00
10	10.000009	10.00000	0.00001	0.000026	2.00
20	20.000031	20.00000	0.00003	0.000037	2.00
30	30.000040	30.00001	0.00003	0.000050	2.00
50	50.000028	50.00002	0.00001	0.000068	2.00
80	80.000068	80.00002	0.00005	0.00011	2.00



## Calibration Report

**Certificate No.:** 2402283-002-01

**Equipment:**

Electronic Balance

**Manufacturer:** METTLER TOLEDO

**Model:** XSR205DU

**Resolution:** 0.00001 g / 0.0001 g

**Serial No.:** C210685394

**ID No.:** UAE.WAO.010/2565

**Capacity:** 220 g

**Date of Calibration:** 2 April 2024

Page 4 of 4

**Calibration Results:** (Continued)

**Calibration Range:** 81 - 200 g

**Calibration Adjustment:** Internal Calibration

**3. Departure from Nominal Value:** (Range: 81 - 200 g ; Resolution: 0.0001 g )

Nominal Value ( g )	Standard Value ( g )	Average Reading ( g )	Correction ( g )	Uncertainty ( ± g )	Coverage Factor <i>k</i>
90	90.00010	90.0001	0.0000	0.00015	2.00
100	100.00006	100.0001	0.0000	0.00015	2.00
110	110.00007	110.0001	0.0000	0.00016	2.00
120	120.00009	120.0000	0.0001	0.00017	2.00
130	130.00010	130.0000	0.0001	0.00019	2.00
140	140.00014	140.0000	0.0001	0.00020	2.00
150	150.00009	150.0001	0.0000	0.00020	2.00
160	160.00010	160.0001	0.0000	0.00022	2.00
170	170.00012	170.0001	0.0000	0.00023	2.00
200	200.00016	200.0002	0.0000	0.00028	2.00

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k* , providing level of confidence of approximately 95 %.

----- End -----

F-CS-012 Revision: 01 Date: 20-04-65

## Calibration Certificate

**Certificate No.:** 2500116-001-01  
**Client name:** UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.  
**Address:** 3 Soi Udomsuk 41, Sukhumvit Road,  
Bangchack, Prakanong, Bangkok 10260

Page 1 of 3

**Equipment:** CHAMBER (Hot Air Oven)

**Manufacturer:** MEMMERT

**Model:** UF55

**Serial No.:** B216.1666

**ID No.:** UAE.WAO.027/2559

**Order No.:** 2500116

**Operation No.:** 2500116-001

**Date of Receipt:** 8 October 2024

**Date of Calibration:** 8 October 2024

**Calibrated by** Mr.Yothin Charoensuk  
Scientist

**Approved by**   
( Mr.Pheraphat Tuanjit )

Manager, Division of Calibration Laboratory

**Date of Issue:** 15 October 2024

Responsible for the Technical Management Team

**The uncertainties are for a confidence probability of approximately 95 %.**

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the National Food Institute.

F-CS-009 Revision: 01 Date: 20-04-65

## Calibration Report

**Certificate No.:** 2500116-001-01

**Equipment:** CHAMBER (Hot Air Oven)

Model: UF55 Serial No.: B216.1666

Resolution: 0.1 °C ID No.: UAE.WAO.027/2559

Manufacturer: MEMMERT

**Date of Calibration:** 8 October 2024

Page 2 of 3

**Location:** Laboratory, UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.

**Environment Condition:**

Ambient Temperature ( 30.3 ± 1 ) °C

Relative Humidity ( 55 ± 1 ) %

Line Voltage ( 230 ± 3 ) Volt

### Condition of this results of Calibration:

- This instrument was calibrated by insert 9 standard thermometer into its chamber and calibration according to W-TE-014 Based on TLAS G-20-1/02-08 (E): Guidelines for Calibration and Checks of Temperature Controlled Enclosures.
  - The temperature scale used was based on ITS - 90.
  - All data show below were final values and the initial data may be obtained upon request.

### 2. Reference Standard Instrument :

Instrument	Model	Serial No./ID No.	Certificate No.	Due Date	Through
Digital Thermometer with sensor	34972A	MY57003188	TE 670486-01	8 June 2025	NATIONAL FOOD INSTITUTE
	RTD	CH#201-209/ RTD#201-209			

- This certificate is traceable to International System of Units (SI Units).
- This certificate was certified only for the instrument we calibrated.
- This result of calibration was found accurate as shown on date and place of calibration only.
- Condition of Calibrated item : Good

### UUC Description :

Time of Record 1 Hour 9 Minute At 104.0,140.0 and 180.0 °C

Fresh air Damper ☐ Open Position ☐

☒ Close Fan 40%

☐ Not Available

7. Result of Calibration : ☒ Without adjustment ☐ After adjustment



## Calibration Report

**Certificate No.:** 2500116-001-01

**Equipment:** CHAMBER (Hot Air Oven)

Model: UF55 Serial No.: B216.1666

Resolution: 0.1 °C ID No.: UAE.WAO.027/2559

Manufacturer: MEMMERT


**Date of Calibration:** 8 October 2024

Page 3 of 3

**Calibration point:** 104.0, 140.0 and 180.0 °C

**Calibration result:**

Calibration Condition	Temperature (°C)	Relative Humidity (%)	Line Voltage (Volt)
MIN	29.3	54	227.0
MAX	31.2	56	232.0

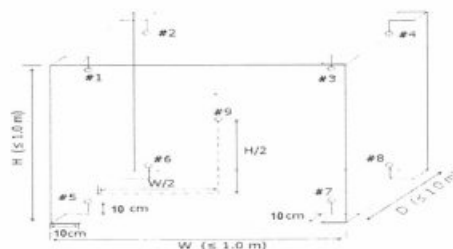

**Table 1 : Reporting of Temperature**

Calibration point (°C)	Measured Temperature (°C) @ Sensor No. (Sensor No.9 is REF)									Uncertainty ± (°C)
	# 1	# 2	# 3	# 4	# 5	# 6	# 7	# 8	# 9	
104.0	103.89	103.66	103.88	103.89	104.40	103.98	103.70	104.10	104.15	0.53
140.0	139.85	139.53	139.87	139.88	140.67	140.00	139.60	140.25	140.23	0.73
180.0	179.63	179.22	179.71	179.76	181.03	180.06	179.41	180.87	180.39	0.90

**Table 2 : Reporting of Characterization Result**

UUC* Setting (°C)	UUC* Reading (°C)			Stability ± (°C)	Uniformity (°C)	Overall Variation (°C)
	MIN	MAX	Average			
104.0	104.0	104.0	104.0	0.15	0.49	0.88
140.0	140.0	140.0	140.0	0.13	0.71	1.2
180.0	180.0	180.0	180.0	0.13	1.2	1.9

**Note** The quoted uncertainty include " Stability " and " Loading effect (20% of Temp Uniformity) "

UUC\* = Unit Under Calibration

Stability = One-half of the greatest maximum difference of measured temperatures at any one sensors, for at least half an hour after reaching steady state.

Uniformity = The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time.

Overall Variation = The difference of the maximum and minimum measured temperatures throughout observation time.

The report uncertainty of measurement was based on standard uncertainty multiplied by coverage factor  $k=2$ , level of confidence of approximately 95 %.

----- End -----



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)  
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES  
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250  
TEL.0-2717-3000-29 FAX.0-2719-9484



## Certificate of Calibration

Cert.No.: 24MM293

Page.: 1 of 3

**Equipment :** Electronic Balance

**Manufacturer :** Mettler Toledo

**Model :** XSR204

**Serial No. :** C117635043

**ID No. :** UAE.WAS.012/2564

**Submitted by :** United Analyst and Engineering Consultant Co.,Ltd.  
3 Soi Udomsuk 41, Sukhumvit Road,  
Bangchak, Phrakhanong,  
Bangkok 10260

**Location :** Balance Room (108)


**Received order :** 11 May 2024

**Calibration Date :** 11 May 2024

**Ambient Temperature :** 15 °C to 40 °C

**Relative Humidity :** 30 % to 90 %

**Calibrated by :** Khit Ruttanaprapachai

**Approved by :**   
Approved Signatory

( ) Ponpan Paipim  
( ) Suwit Imjai  
(✓) Kunchit Promprat

**Issue Date :** 15 May 2024

**The Uncertainties are for a confidence probability of approximately 95%**

This certificate may not be reproduced other than in full, except with the prior written  
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

เอกสารไม่ควบคุม





Equipment : Electronic Balance  
Condition As-Received : Used Item  
Reference : 2405-0166OC-2

Cert.No.: 24MM293

Page: 2 of 3

**Procedure used :-**

Calibration were conducted using in-house calibration procedure CP-OB01 based on UKAS LAB 14 according to direct measurement method against standard weight.

**Condition of this result of calibration**

1. Reference standard instruments:-

<u>Instruments</u>	<u>Model</u>	<u>Serial No.</u>	<u>ID No.</u>	<u>Test report No.</u>	<u>Due date</u>
1) Standard Weight Set (E2)	15884	24053	70RC007	MM-0013-24	25 Jan 2026

2. This certificate is valid only to the item calibrated on date and place of calibration.
3. This result of calibration was made on requested at the point specified by customer.
4. This certificate is not certified for any commercial transaction.
5. This certification is traceable to the International System of Unit.

**Result of calibration** ( ) Without Adjustment ( \* ) After Adjustment by Internal Calibration

**Range capacity :** 0 g to 220 g **Resolution** 0.0001 g

**Before Adjustment :**

<u>Applied Weight</u>	<u>Balance Reading</u>	<u>Correction</u>	<u>Measurement Uncertainty</u>	<u>Coverage Factor</u>
( g )	( g )	( g )	( $\pm$ mg )	( k )
100	100.0000	0.0000	0.27	2.03
200	200.0001	-0.0001	0.31	2

**After Adjustment :**

1. **Determination of the standard deviation of weighing machine** ( n = 10 )

<u>Applied Weight</u>	<u>Standard Deviation of Reading ( g )</u>
( g )	
100	0.00007
200	0.00007



Equipment : Electronic Balance  
Condition As-Received : Used Item  
Reference : 2405-0166OC-2


Cert.No.: 24MM293

Page: 3 of 3

### Result of calibration

#### 2. Effect of off center loading

A mass of 100 g was placed to various position on the pan.  
The weighing machine reading error obtained is given in the table

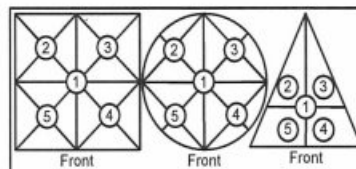

Maximum difference between  
off-center and central loading

Position 1	Position 2	Position 3	Position 4	Position 5
( g )	( g )	( g )	( g )	( g )
+0.0002	-0.0001	0.0000	+0.0002	0.0000

( g )  
0.0003

#### 3. Departure from nominal value

Applied Weight	Balance Reading	Correction	Measurement Uncertainty	Coverage Factor
( g )	( g )	( g )	( ± mg )	( k )
Unload	0.0000	0.0000	0.15	2.13
1	1.0000	0.0000	0.15	2.13
5	5.0000	0.0000	0.15	2.13
10	10.0000	0.0000	0.15	2.11
20	20.0000	0.0000	0.19	2.03
50	50.0001	-0.0001	0.19	2.06
60	60.0001	-0.0001	0.19	2.04
80	80.0001	-0.0001	0.27	2
100	100.0002	-0.0002	0.27	2.03
120	120.0001	-0.0001	0.29	2
200	200.0001	-0.0001	0.31	2

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor  $k$ , providing a level of confidence of approximately 95 %.

-o0o-





TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)  
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES  
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250  
TEL. 0-2717-3000-29 FAX. 0-2719-9484



Cert. No.: 24TM303

Page : 1 of 3

## Certificate of Calibration

**Equipment :** BOD Incubator

**Manufacturer :** Arco

**Model :** UC4-1320

**Serial No. :** 13URC4S013201

**ID No. :** UAE.WAO.015/2561

**Submitted by :** United Analyst and Engineering Consultant Co.,Ltd.  
3 Soi Udomsuk 41, Sukhumvit Road,  
Bangchak, Phrakhanong,  
Bangkok 10260

**Location :** Lab Floor 2

**Received Order :** 10 February 2024

**Calibration Date :** 10 February 2024

**Ambient Temperature :** ( 26 ± 10 ) °C

**Relative Humidity :** ( 50 ± 30 ) %

**Calibrated by :** Tawatchai Pama

**Approved by :**

Approved Signatory

- ( ) Pornthippa Tameyakul  
( ✓ ) Unnopphol Harachai  
( ) Suwit Imjai

**Issue Date :** 19 February 2024

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written  
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

เอกสารไม่ควบคุม



Equipment : BOD Incubator  
Condition As-Received : Used Item  
Reference : 2402-0234OC-1  
Result of Calibration :- ( \* ) Without Adjustment  
Function of UUC\* : Temperature Source  
Fresh air setting : Not Available

Cert. No.: 24TM303

Page : 3 of 3

Calibration Point ( °C )	UUC* Setting ( °C )	UUC* Reading ( °C )	Temperature stability ( ± °C )	Temperature uniformity ( °C )	Overall Variation ( °C )	Coverage Factor <i>k</i>
20.0	20.1	19.9	0.37	0.72	1.4	2

Calibration Point ( °C )	Measured Temperature ( °C )									Uncertainty  ( ± °C )
	Position									
	1	2	3	4	5	6	7	8	9 (ref.)	
20.0	19.873	19.803	20.322	19.690	19.615	19.585	19.612	19.558	19.645	0.58

**Average\*** : The average of 30 values in each position.

**Temperature stability** : One-half of the greatest maximum difference of measured temperature at any one sensor.

**Temperature uniformity** : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.

**Overall Variation** : The Difference of the maximum and minimum measured temperatures throughout observation.

**UUC\*** : Unit Under Calibration

Note : The reported uncertainty of measurement was included stability and excluded uniformity .

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-





Equipment : BOD Incubator  
Condition As-Received : Used Item  
Reference : 2402-0234OC-1

Cert. No.: 24TM303

Page : 2 of 3

**Procedure Used :-**

Calibration were conducted using calibration procedure CP-OT02 based on TLAS G-20 according to direct measurement method with Data Acquisition which connected with Resistance Temperature Detector ( RTD ).

The temperature scale used was based on ITS-90.

**Condition of this result of calibration**

1. Reference standard instrument:-

<u>Instrument</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Traceable</u>	<u>Due Date</u>
1 ) Data Acquisition	MY59003411	23LM208	TPA	27 Dec 2024

2. This certificate is valid only to the item calibrated on date and place of calibration.


3. This certification is traceable to the International System of Unit.

**Remark :** TPA : Technology Promotion Association ( Thailand - Japan )

**Result of Calibration :-** ( \* ) Without Adjustment

**Function of UUC\* :** Temperature Source

**Fresh air setting :** Not Available

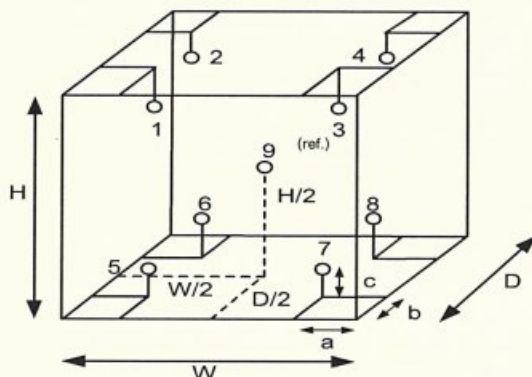

Environment during calibration		
	Beginning	Finished
Temp. ( °C )	28	31
REL.Humid. ( % )	70	65
AC Supply ( Volt )	233	234

Position :	Ref. Std. ID No.:
1	20RTD-2/1
2	20RTD-2/2
3	20RTD-2/3
4	20RTD-2/4
5	20RTD-2/5
6	20RTD-2/6
7	20RTD-2/7
8	20RTD-2/8
9 (ref.)	20RTD-2/9

**Probe Installation Details :**

a = 10 cm  
b = 10 cm  
c = 10 cm

**Dimension of Chamber :**

D = 0.62 m  
W = 1.2 m  
H = 1.2 m  
Capacity = 0.89 m<sup>3</sup>



**TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)**  
**CORPORATE SERVICES 3 : EQUIPMENT CALIBRATION AND TESTING SERVICES**



534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250

TEL. 0-2717-3000 FAX. 0-2719-9484

**Cert.No.:** 24TW39

**Page.:** 1 of 2

## Certificate of Testing

<b>Equipment :</b>	DO Meter
<b>Manufacturer :</b>	YSI
<b>Model :</b>	5100
<b>Serial No. :</b>	11B 101863
<b>ID No. :</b>	UAE.WAO.004/2554
<b>Received Date :</b>	20 February 2024
<b>Test Date :</b>	21 February 2024
<b>Reference :</b>	2402-0629DSC-1
<b>Submitted by :</b>	United Analyst and Engineering Consultant Co.,Ltd. 3 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
<b>Laboratory Condition :</b>	Temperature ( $25 \pm 5$ ) °C Humidity ( $50 \pm 20$ ) %
<b>Test Procedure :</b>	In - house method : CP-CH9 by Comparison Technique with Azide Modification Method
<b>Tested by :</b>	Walalak Sirithean 
<b>Approved by :</b>	 Approved Signatory
( ) Pornthippa Tameyakul	
( ) Unnopphol Harachai	
( <input checked="" type="checkbox"/> ) Saithip Meangmai	

**Issue Date :** 22 February 2024

**เอกสารไม่ควบคุม**





Cert.No.: 24TW39

Page.: 2 of 2

**Condition of this result of calibration**

1. Reference Standard Instruments :

This certification is traceable to the International System of Unit through the reference standards laboratory of Industrial Calibration Center, Technology Promotion Association (Thailand-Japan).

<u>Instruments</u>	<u>Serial No.</u>	<u>ID No.</u>	<u>Certificate No.</u>	<u>Due Date</u>
1. Burette	-	130BU10	23CG1172	22 Mar 2025
2. Balance	14233821	110RC001	23MM405	16 July 2024

2. Standard Material :-

<u>Material</u>	<u>Manufacturer</u>	<u>Lot.No.</u>	<u>Assay</u>
Sodium Thiosulfate pentahydrate	Merck	AM1763316	100.2%

**Result :** Dissolved Oxygen Meter Adjustment With Air 100 %

Dissolved Oxygen Probe No.: 22B100125

<b>Titration Method (Azide Modification Method)</b> (mg/L)	<b>DO Meter Reading</b> (mg/L)	<b>Standard Deviation</b> (mg/L)
8.20	8.19	0.0055

This report was certified only for the instrument we tested. It is allowable to use for study  
Intend to use for advertising and referral purpose is prohibited. This report may not be reproduced  
other in full, without written approval of the laboratory

-o0o-

เอกสาร


Certificate No. : HIT-2417-0568

Page : 1 of 2

**CERTIFICATE OF CALIBRATION**

<b>Equipment :</b>	COD Test Tube Heater		
<b>Meter Model :</b>	HI839800-02	<b>Serial No. :</b>	1147807
<b>Tube Heater :</b>	25 Vial Capacity	<b>Resolution :</b>	0.1°C
<b>Temperature Range :</b>	(-10 to 160)°C	<b>Temperature of Reaction :</b>	150°C
<b>Manufacturer :</b>	Hanna Instruments	<b>Made in :</b>	Romania
<b>Condition As-Received :</b>	Used Product	<b>Reference :</b>	RE240681
<b>Ambient Temperature :</b>	(25 ± 2)°C	<b>Relative Humidity :</b>	(50 ± 15)%RH
<b>Customer name :</b>	United Analyst and Engineering Consultant Co., Ltd. 3 Soi Udomsuk 41, Sukhumvit Rd., Bangchak, Phrakhanong, Bangkok 10260		
<b>Received date :</b>	22 April 2024		
<b>Calibrate date :</b>	23 April 2024		
<b>Issue date :</b>	25 April 2024		
<b>Calibrated Location :</b>	Hanna Instruments (Thailand) Ltd.		
<b>Calibration Procedure :</b>	This calibrator was conducted by using in-house: calibration procedure CP-04 by using certified reference standard instruments.		

**Calibrated by :** ☒ Mr. Pichit Petthong  
☐ Mr. Channarong Soinak

**Approved by :**   
Mr. Anan Suwanchaisakul  
Authorized Signatory



This certificate was certified only for the instrument we calibrated.

This result of calibration was found accurate on date and place of calibration only.

\*\* This certificate may not be reproduced other than in full, except with the prior written \*\*  
approval of the head of Hanna Instrument (Thailand).

เอกสารไม่ควบคุม

**Condition of this calibration result:**

Reference Standard Instruments : This certification is traceable to the international unit of unit maintained through:

Instruments	Model	Serial No.	Certificate No.	Traceable
Data Acquisition Switch Unit	34970A	MY44065265	WK2307-164-1	WK Electric Co., Ltd.
Digital Thermo-Hygrometer	HT-771SD	AI.07155	24H41	Technology Promotion Association (Thailand-Japan).

**Calibration Result:**

Measurement Temperature Source Accuracy for COD Reactor.

Capacity (Vial)	Nominal Value (°C)	Average Value (°C)	Uncertainty of Measurement (±°C)
25 Vial	150.0	149.8	0.49

Unit : °C

(1A) 148.901	(2A) 149.249	(3A) 149.950	(4A) 150.042	(5A) 149.186
(1B) 149.724	(2B) 149.578	(3B) 149.852	(4B) 150.100	(5B) 150.117
(1C) 149.863	(2C) 149.799	(3C) 150.233	(4C) 149.847	(5C) 149.977
(1D) 149.550	(2D) 149.666	(3D) 149.958	(4D) 149.744	(5D) 149.819
(1E) 150.044	(2E) 149.869	(3E) 149.361	(4E) 149.973	(5E) 149.654

Figure: Shows the location of the temperature source.

The report uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor  $k = 2$ , providing a level of confidence of approximately 95%


\*\* End of certificate \*\*



## CERTIFICATE OF CALIBRATION

**Certificate No. :** SP24-018

Page 1 of 5

**Customer :** United Analyst and Engineering Consultant Co.,Ltd. (Head Office)**Address :** 3 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260**Location of calibration :** Laboratory 315**Equipment :** UV-Vis Spectrophotometer**Manufacturer :** Agilent Technologies**Model :** Cary 60**Serial No. :** MY15410009**ID No. :** UAE.WAT.020/2558**Received Date :** 7 May 2024**Calibration Date :** 7 May 2024**Issue Date :** 9 May 2024**Condition Instrument :** Good**Calibrated by :**  
( Mr.Tanawut Rittidach )

Technical Manager

**Approved by :**  
( Ms. Chonthicha Sangngern )

Quality Manager

The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only.

The measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the DQE Services Co., Ltd.

## REPORT OF CALIBRATION

**Certificate No. :** SP24-018

Page 2 of 5

**Environment Condition :** Ambient Temperature  $25 \pm 5$  °CRelative humidity  $55 \pm 20$  %RH**Calibration method :** In-house method CP-01 Based on ASTM E275-08**Certified Reference Materials :**

Material	Serial No.	Certificate No.	Due date
Absorbance Standard set	25760	115663	25 October 2025
Absorbance Standard set	25757	115638	25 October 2025
Wavelength Standard set	25806	115657	25 October 2025
Wavelength Standard set	25758	115665	25 October 2025

**Traceability :** This certification is traceable to the International System of Unit maintained at National -

Institute of Standards and Technology (NIST) through Sarna Scientific Limited

**Spectral Band Width of UUC :** 1.5 nm.**Scan Speed of UUC :** 60 nm/min**Scan Interval of UUC :** 0.15 nm.**Resolution of UUC :** Photometric 0.0001 Abs.

Wavelength 0.1 nm.

## REPORT OF CALIBRATION

Certificate No. : SP24-018

Page 3 of 5

Calibration Results : Without adjustment

Photometric Accuracy :

Wavelength (nm.)	CRMs Values (Abs)	UUC Reading (Abs)	Correction (Abs)	Uncertainty (Abs)	Coverage factor <i>k</i>
420	0.0000	0.0000	0.0000	0.0028	2.00
	0.5780	0.5747	0.0033	0.0031	2.00
	1.0484	1.0438	0.0046	0.0029	2.00
	2.1876	2.1832	0.0044	0.0080	2.00
440	0.0000	0.0000	0.0000	0.0028	2.00
	0.5595	0.5581	0.0014	0.0034	2.00
	1.0239	1.0231	0.0008	0.0035	2.00
	2.1230	2.1219	0.0011	0.0080	2.00
465	0.0000	0.0000	0.0000	0.0028	2.00
	0.5230	0.5184	0.0046	0.0030	2.00
	0.9633	0.9614	0.0019	0.0029	2.00
	1.9753	1.9731	0.0022	0.0070	2.00
546.1	0.0000	0.0000	0.0000	0.0028	2.00
	0.5181	0.5150	0.0031	0.0031	2.00
	1.0002	0.9964	0.0038	0.0033	2.00
	1.9973	1.9914	0.0059	0.0088	2.00
590	0.0000	0.0000	0.0000	0.0028	2.00
	0.5517	0.5485	0.0032	0.0030	2.00
	1.0803	1.0772	0.0031	0.0030	2.00
	2.0373	2.0293	0.0080	0.0080	2.00
635	0.0000	0.0000	0.0000	0.0028	2.00
	0.5591	0.5565	0.0026	0.0031	2.00
	1.0518	1.0482	0.0036	0.0030	2.00
	1.9274	1.9202	0.0072	0.0079	2.00



## REPORT OF CALIBRATION

Certificate No. : SP24-018

Page 4 of 5

### Photometric Accuracy :

Wavelength (nm.)	CRMs Values (Abs)	UUC Reading (Abs)	Correction (Abs)	Uncertainty (Abs)	Coverage factor <i>k</i>
235	0.0000	0.0000	0.0000	0.0050	2.00
	0.7469	0.7435	0.0034	0.0057	2.00
257	0.0000	0.0000	0.0000	0.0050	2.00
	0.8674	0.8639	0.0035	0.0060	2.00
313	0.0000	0.0000	0.0000	0.0050	2.00
	0.2919	0.2907	0.0012	0.0051	2.00
350	0.0000	0.0000	0.0000	0.0050	2.00
	0.6430	0.6402	0.0028	0.0055	2.00

## REPORT OF CALIBRATION

Certificate No. : SP24-018

Page 5 of 5

### Wavelength Accuracy :

CRMs Values (nm.)	UUC Reading (nm.)	Correction (nm.)	Uncertainty (nm.)	Coverage factor <i>k</i>
241.72	242.0	-0.28	0.18	2.00
279.45	279.5	-0.05	0.18	2.00
287.81	287.9	-0.09	0.18	2.00
334.06	333.9	0.16	0.18	2.00
360.93	360.5	0.43	0.18	2.00
418.59	418.1	0.49	0.18	2.00
445.94	445.6	0.34	0.18	2.00
453.66	453.3	0.36	0.18	2.00
460.02	459.8	0.22	0.18	2.00
536.59	536.0	0.59	0.18	2.00
637.98	638.7	-0.72	0.18	2.00
431.38	430.8	0.58	0.18	2.00
472.50	472.4	0.10	0.18	2.00
513.47	513.7	-0.23	0.18	2.00
528.88	529.1	-0.22	0.18	2.00
573.17	573.5	-0.33	0.18	2.00
585.35	585.2	0.15	0.20	2.00
684.40	685.1	-0.70	0.18	2.00
740.72	741.4	-0.68	0.20	2.00
748.55	749.1	-0.55	0.18	2.00
807.03	807.3	-0.27	0.18	2.00
879.28	879.3	-0.02	0.18	2.00

Remark : - UUC = Unit Under Calibration

- N/A = Not Available

- The result expanded uncertainty of measurement  $U$  is stated as the standard uncertainty of measurement multiplied by the coverage factor  $k$ ,

which for a normal distribution corresponds to a coverage probability of approximately 95%

- \* Indicates non TISI accredited

- End of Certificate -

**เอกสารไม่ควบคุม**  
 FM-708-02 R01 1/11/2021



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)  
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES  
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250  
TEL.0-2717-3000-29 FAX.0-2719-9484



## Certificate of Calibration

Cert. No.: 24TM648

Page : 1 of 3

Equipment : Incubator  
Manufacturer : Memmert  
Model : IPP 260  
Serial No. : V615.0187  
ID No. : UAE.MIC.003/2559  
Submitted by : United Analyst and Engineering Consultant Co.,Ltd.  
3 Soi Udomsuk 41, Sukhumvit Road,  
Bangchak, Phrakhanong,  
Bangkok 10260  
Location : Microbiology Laboratory  
Received Order : 01 April 2024  
Calibration Date : 01 April 2024  
Ambient Temperature : (  $26 \pm 10$  ) °C  
Relative Humidity : (  $50 \pm 30$  ) %

Calibrated by : Man Pattanapongpaiboon

Approved by :

Approved Signatory

( ) Ponpan Paipim  
(✓) Suwit Imjai  
( ) Kunchit Promprat

Issue Date :

7 April 2024

**The Uncertainties are for a confidence probability of approximately 95%**

This certificate may not be reproduced other than in full, except with the prior written  
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

เอกสารไม่ควบคุม





Equipment : Incubator  
Condition As-Received : Used Item  
Reference : 2404-0003OC-1

Cert. No.: 24TM648

Page : 2 of 3

**Procedure Used :-**

Calibration were conducted using calibration procedure CP-OT02 based on TLAS G-20 according to direct measurement method with Data Acquisition which connected with Resistance Temperature Detector ( RTD ).

The temperature scale used was based on ITS-90.

**Condition of this result of calibration**

1. Reference standard instrument:-

<u>Instrument</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Traceable</u>	<u>Due Date</u>
1 ) Data Acquisition	MY49023932	23LM122	TPA	26 Jul 2024

2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certification is traceable to the International System of Unit.


**Remark :** TPA : Technology Promotion Association ( Thailand - Japan )

**Result of Calibration :-** ( \* ) Without Adjustment

**Function of UUC\* :** Temperature Source

**Fresh air setting :** Close

Environment during calibration		
	Beginning	Finished
Temp. ( °C )	24	24
REL.Humid. ( % )	54	57
AC Supply ( Volt )	221	223

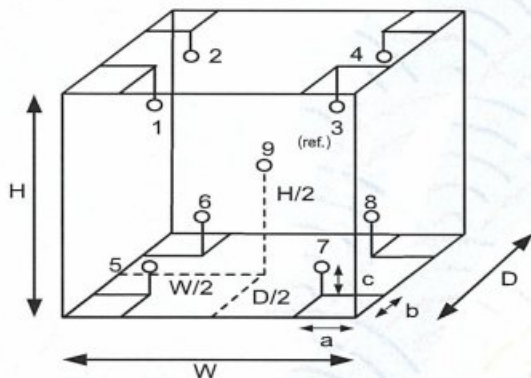

Position :	Ref. Std. ID No.:
1	19-16RTD-01
2	19-16RTD-02
3	19-16RTD-03
4	19-16RTD-04
5	19-16RTD-05
6	19-16RTD-06
7	21-16RTD-07
8	19-16RTD-08
9 (ref.)	19-16RTD-09

**Probe Installation Details :**

a = 5.0 cm  
b = 5.0 cm  
c = 5.0 cm

**Dimension of Chamber :**

D = 0.50 m  
W = 0.64 m  
H = 0.80 m  
Capacity = 0.26 m<sup>3</sup>



Equipment : Incubator  
Condition As-Received : Used Item  
Reference : 2404-0003OC-1  
Result of Calibration :- ( \* ) Without Adjustment  
Function of UUC\* : Temperature Source  
Fresh air setting : Close

Cert. No.: 24TM648

Page : 3 of 3

Calibration Point ( °C )	UUC* Setting ( °C )	UUC* Reading ( °C )	Temperature stability ( ± °C )	Temperature uniformity ( °C )	Overall Variation ( °C )	Coverage Factor <i>k</i>
35.0	35.0	35.0	0.028	0.13	0.24	2

Calibration Point ( °C )	Measured Temperature ( °C )									Uncertainty ( ± °C )
	Position									
	1	2	3	4	5	6	7	8	9 (ref.)	
35.0	34.908	35.004	34.989	35.099	35.089	35.095	34.921	34.936	35.002	0.30

**Average\*** : The average of 30 values in each position.

**Temperature stability** : One-half of the greatest maximum difference of measured temperature at any one sensor.

**Temperature uniformity** : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.

**Overall Variation** : The Difference of the maximum and minimum measured temperatures throughout observation.

**UUC\*** : Unit Under Calibration

**Note** : The reported uncertainty of measurement was included stability and excluded uniformity .

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-





TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)  
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES  
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250  
TEL. 0-2717-3000-29 FAX. 0-2719-9484



Cert. No.: 24TM29

Page : 1 of 3

## Certificate of Calibration

**Equipment :** Water Bath

**Manufacturer :** Memmert

**Model :** WNE 14

**Serial No. :** L416.0606

**ID No. :** UAE.MIC.002/2560

**Submitted by :** United Analyst and Engineering Consultant Co.,Ltd.  
3 Soi Udomsuk 41, Sukhumvit Road,  
Bangchak, Phrakhanong,  
Bangkok 10260

**Location :** Microbiology Laboratory

**Received Order :** 10 February 2024

**Calibration Date :** 10 February 2024

**Ambient Temperature :** ( 26 ± 10 ) °C

**Relative Humidity :** ( 50 ± 30 ) %

**Calibrated by :** Krisda Malee

**Approved by :**

Approved Signatory

- ( ) Pornthippa Tameyakul  
( ✓ ) Unnopphol Harachai  
( ) Suwit Imjai

**Issue Date :** 19 February 2024

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written  
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

เอกสารไม่ควบคุม





**Equipment :** Water Bath  
**Condition As-Received :** Used Item  
**Reference :** 2402-0232OC-2

**Cert. No.:** 24TM29

**Page :** 2 of 3

**Procedure Used :-**

Calibration were conducted using in-house calibration procedure CP-OT04 Based on ASTM E715 according to direct measurement method with Data Acquisition which connected with Industrial Platinum Resistance Thermometer ( IPRT ).

The temperature scale used was based on ITS-90.

**Condition of this result of calibration**

1. Reference standard instrument:-

<u>Instrument</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Traceable</u>	<u>Due Date</u>
1 ) Data Acquisition	MY49001451	23LM27	TPA	25 Feb 2024

2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certification is traceable to the International System of Unit.


**Remark :** TPA : Technology Promotion Association ( Thailand - Japan )

**Result of Calibration :-** ( \* ) Without Adjustment

**Function of UUC\* :** Temperature Source

**Heat transfer medium used :** Water

	Environmental		AC Voltage Supply
	( °C )	( %R.H. )	( Volt )
Beginning of Calibration	26	51	220
Finished of Calibration	25	50	221

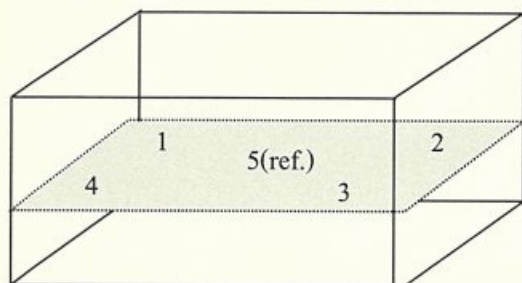

Front

Position :	Ref. Std. ID No.:
1	N37P301419
2	N37P300732
3	N37P301420
4	N37P301421
5(ref.)	N37P301425



Equipment : Water Bath  
Condition As-Received : Used Item  
Reference : 2402-0232OC-2  
Result of Calibration :- ( \* ) Without Adjustment  
Function of UUC\* : Temperature Source

Cert. No.: 24TM29

Page : 3 of 3

Calibration point ( °C )	UUC* Setting ( °C )	UUC* Reading ( °C )	Average* Standard Reading ( °C )					Uncertainty  ( ± °C )
			Position					
			1	2	3	4	5 (ref.)	
44.5	44.4	44.4	44.508	44.469	44.502	44.521	44.527	0.15

Calibration point ( °C )	Uniformity ( °C )	Stability ( ± °C )	Coverage Factor <i>k</i>
44.5	0.15	0.074	2

**Average\*** : The average of 30 values in each position.

**Uniformity** : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.

**Stability** : One-half of the greatest maximum difference of measured temperature at any one probe.

**UUC\*** : Unit Under Calibration

**Note** : The reported uncertainty of measurement was included stability and excluded uniformity.

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-oOo-

เอกสาร



## Calibration Certificate

**Certificate No.:** 2402281-001-01  
**Client name:** UNITED ANALYST AND ENGINEERING CONSULTANT CO., LTD.  
**Address:** 3 Soi Udomsuk 41, Sukhumvit Road,  
Bangchack, Prakhnong, Bangkok 10260

Page 1 of 3

**Equipment:** Autoclave  
**Manufacturer:** ALP  
**Model:** CL-40L  
**Serial No.:** 808763  
**ID No.:** UAE.MIC.026/2563  
**Order No.:** 2402281  
**Operation No.:** 2402281-001  
**Date of Receipt:** 2 April 2024  
**Date of Calibration:** 2 April 2024

**Calibrated by** Mr.Jerawut Prapawuttipong  
Scientist

**Approved by**

( Mr.Pheraphat Tuanjit )

Manager, Division of Calibration Laboratory

**Date of Issue:** 9 April 2024

Responsible for the Technical Management Team

**The uncertainties are for a confidence probability of approximately 95 %.**

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the National Food Institute.

F-CS-009 Revision: 01 Date: 20-04-65



## Calibration Report

**Certificate No.:** 2402281-001-01  
**Equipment:** Autoclave  
Model: CL-40L Serial No.: 808763  
Resolution: 0.1 °C ID No.: UAE.MIC.026/2563  
Manufacturer: ALP  
**Date of Calibration:** 2 April 2024

Page 2 of 3

**Location:** LABORATORY, UNITED ANALYST AND ENGINEERING CONSULTANT CO., LTD.  
**Environment Condition:** Ambient Temperature ( 25 ± 1 ) °C  
Relative Humidity ( 55 ± 7 ) %  
Line Voltage ( 225 ± 5 ) Volt

### Condition of this results of Calibration:

- This instrument was calibrated by insert 3 standard temperature recorder with RTD into its autoclave and calibration according to W-TE-018 based on BS 2646-1(2021) : Autoclaves for sterilization in laboratories Design, construction, safety and performance Specification.  
- The temperature scale used was based on ITS - 90 .  
- All data show below were final values and the initial data may be obtained upon request.

### 2. Reference Standard Instrument :

Instrument	Model	Serial No.	Certificate No.	Due Date	Through
Digital Thermometer with RTD (Data Logger)	HiTemp140-2	R54918	TE 660383-01	8 April 2024	NATIONAL FOOD INSTITUTE
	HiTemp140-2	S25601	TE 670033-01	9 November 2024	MADGETECH INC.
	HiTemp140-2	S25602	TE 670034-01	9 November 2024	MADGETECH INC.

- This certificate is traceable to International System of Units (SI Units).
- This certificate was certified only for the instrument we calibrated.
- This result of calibration was found accurate as shown on date and place of calibration only.
- This standard does not apply to sterilizers or disinfectors used for medical, dental, pharmaceutical.
- Condition of Calibrated item : Good

UUC Description : Setting program function sterilization : STERILIZE/NORMAL

Time of sterilization 15 Minute At 115.0 and 121.0 °C

8. Result of Calibration : ☒ Without adjustment  
☐ After adjustment

## Calibration Report

**Certificate No.:** 2402281-001-01  
**Equipment:** Autoclave  
Model: CL-40L Serial No.: 808763  
Resolution: 0.1 °C ID No.: UAE.MIC.026/2563  
Manufacturer: ALP


**Date of Calibration:** 2 April 2024

Page 3 of 3

**Calibration point:** 115.0 and 121.0 °C

**Calibration result:**

Calibration Condition	Temperature (°C)	Relative Humidity (%)	Line Voltage (Volt)
Min	24.4	48.6	220
Max	25.5	62.1	230

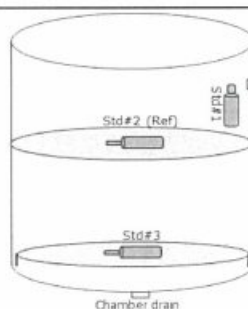

Standard at Position

Std#1 = Attached to the load temperature probe, within 20 mm.  
Std#2 = In the upper half of the chamber  
Std#3 = In the chamber drain, within 100 mm.

Table1 : Reporting of Temperature

Calibration Point (°C)	Measured Temperature (°C) @ Sensor No. (Sensor No.2 is REF)			Uncertainty ± (°C)
	Std.# 1	Std.# 2 (Ref)	Std.# 3	
115.0	115.28	115.35	115.38	0.64
121.0	121.28	121.36	121.37	0.64

Table 2 : Reporting of Characterization Result

UUC* Setting (°C)	UUC* Reading				Stability ± (°C)	Uniformity (°C)	Overall Variation (°C)
	Min (°C)	Max (°C)	Average (°C)	MPa			
115.0	115.0	115.1	115.0	0.08	0.19	0.13	0.48
121.0	121.0	121.1	121.0	0.12	0.17	0.10	0.38

### Note

The quoted uncertainty include " Stability " and " Loading effect ( 20% of Uniformity )"

UUC\* = Unit Under Calibration

Stability = One-half of the greatest maximum difference of measured temperatures at any one sensors, for at least half an hour after reaching steady state.

Uniformity = The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time.

Overall Variation = The difference of the maximum and minimum measured temperatures throughout observation time.

The report uncertainty of measurement was based on standard uncertainty multiplied by coverage factor k= 2 at a level of confidence of approximately 95 %.

----- End -----



## Calibration Certificate

**Certificate No.:** 2402419-001-01  
**Client name:** UNITED ANALYST AND ENGINEERING CONSULTANT CO., LTD.  
**Address:** 3 Soi Udomsuk 41, Sukhumvit Road,  
Bangchack, Prakhonong, Bangkok 10260

Page 1 of 3

**Equipment:** Electronic Balance  
**Manufacturer:** OHAUS  
**Model:** PX623  
**Serial No.:** C236754745  
**ID No.:** UAE.MIC.055/2565  
**Order No.:** 2402419  
**Operation No.:** 2402419-001  
**Date of Receipt:** 19 April 2024  
**Date of Calibration:** 19 April 2024

**Calibrated by** Mr.Pheraphat Tuanjit  
Scientist

**Approved by**   
( Miss Preeyaporn Jaengkarnkit )

Vice President, Department of Laboratory Services  
Responsible for the Technical Management Team

**Date of Issue:** 23 April 2024

**The uncertainties are for a confidence probability of approximately 95%**

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the National Food Institute.

F-CS-009 Revision: 01 Date: 20-04-65



## Calibration Report

**Certificate No.:** 2402419-001-01

**Equipment:**

Electronic Balance

**Manufacturer:** OHAUS

**Model:** PX623

**Resolution:** 0.001 g

**Serial No.:** C236754745

**ID No.:** UAE.MIC.055/2565

**Capacity:** 620 g

**Date of Calibration:** 19 April 2024

Page 2 of 3

**Environment Condition:** Ambient Temperature: 26.0 ± 0.3 °C Relative Humidity: 57 ± 8.4 %

**Place of Calibration:** Room 301, UNITED ANALYST AND ENGINEERING CONSULTANT CO., LTD.

**Condition of Equipment:** Good Condition

### Condition of This Results of Calibration:

1. Calibration Method: NFI Method W-MA-001 In-House Method based on UKAS Lab 14 : 2019

2. Reference Standards:

Reference Standard	Model	Serial No.	Calibrated By	Certificate No.	Due Date
Standard Weight Class E2	1-500g	15882	TCS	M23111825	28 November 2024

Instrument	Model	Serial No.	Calibrated By	Certificate No.	Due Date
Thermo-Hygro Meter	608-H1	NFI.BTH 019/23	Quality Reborn	QR24-0492	4 March 2025

3. This certification is traceable to SI UNIT

4. This certificate was certified only for the instrument we calibrated.

5. This result of calibration was found accurate as shown on date and place of calibration only.

### Calibration Results:




#### 1. Repeatability of Reading:

Nominal Value ( g )	Standard Deviation of Reading ( g )
300	0.00067
600	0.0010

#### 2. Off-Center Error:

A mass of 200 g was placed and moved to various position on pan.

The balance reading obtained is given in the table.



1 ( g )	2 ( g )	3 ( g )	4 ( g )	5 ( g )	6 ( g )	(Maximum Difference) ( g )
200.000	200.002	200.001	199.999	200.000	200.000	0.002

23 April 2024

## Calibration Report

**Certificate No.:** 2402419-001-01

**Equipment:** Electronic Balance

**Manufacturer:** OHAUS

**Model:** PX623

**Resolution:** 0.001 g

**Serial No.:** C236754745

**ID No.:** UAE.MIC.055/2565

**Capacity:** 620 g

**Date of Calibration:** 19 April 2024

Page 3 of 3

**Calibration Results:** (Continued)

**Calibration Range:** 0-600 g

**Calibration Adjustment:** Internal Calibration

### 3. Departure from Nominal Value:

Nominal Value ( g )	Standard Value ( g )	Average Reading ( g )	Correction ( g )	Uncertainty ( ± g )	Coverage Factor <i>k</i>
Unload	0.0000	0.000	0.000	0.00093	2.00
1	1.0000	1.000	0.000	0.00093	2.00
5	5.0000	5.000	0.000	0.00093	2.00
10	10.0000	10.000	0.000	0.00093	2.00
20	20.0000	20.000	0.000	0.00093	2.00
50	50.0000	50.001	-0.001	0.00093	2.00
100	100.0000	100.001	-0.001	0.00094	2.00
200	200.0000	200.001	-0.001	0.0011	2.00
300	300.0000	300.003	-0.003	0.0011	2.00
400	399.9999	400.003	-0.003	0.0012	2.00
500	499.9999	500.003	-0.003	0.0013	2.00
600	599.9999	600.002	-0.002	0.0014	2.00

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

----- End -----

F-CS-012 Revision: 01 Date: 20-04-65