เอกสารแนบ 17
เอกสารอนุญาตห้องปฏิบัติการ

MM-C20

เอกสารแนบท้ายหนังสือรับต่ออายุขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน
บริษัท ตรวจวัดสิ่งแวดล้อม จำกัด เลขทะเบียน ว-๓๐๑
ที่ อก ๐๓๑๐(๑)/ ๒๖๔๓ ลงวันที่ ๓๑ มกราคม ๒๕๖๖

ขอบข่ายสารมลพิษที่ได้รับขึ้นทะเบียนจากกรมโรงงานอุตสาหกรรม จำนวน ๔ รายการ

น้ำเสีย จำนวน 4 รายการ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
1	Biochemical Oxygen Demand	5-Day BOD Test, Membrane Electrode Method
2	pH	Electrometric Method
3	Total Dissolved Solids	Dried at 180 °C
4	Total Suspended Solids	Dried at 103-1

เอกสารอ้างอิง

APHA, AWWA, WEF. **Standard Methods for the Examination of Water and Wastewater.** 23rd ed. Washington, DC: APHA, 2017.

น.17/1

ที่ อก ๐๓๑๐(๑)/ ๒๖๔๓

กรมโรงงานอุตสาหกรรม
ถนนพระรามที่ ๖ แขวงทุ่งพญาไท
เขตราชเทวี กรุงเทพฯ ๑๐๔๐๐

๓๑ มกราคม ๒๕๖๖

เรื่อง ต่ออายุหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน

เรียน กรรมการผู้จัดการ บริษัท ตรวจวัดสิ่งแวดล้อม จำกัด

อ้างถึง คำขอขึ้นทะเบียน/ต่ออายุ/เปลี่ยนแปลงบุคลากร และชนิดสารมลพิษของห้องปฏิบัติการวิเคราะห์เอกชน ลงวันที่ ๘ ธันวาคม ๒๕๖๕

สิ่งที่ส่งมาด้วย เอกสารแนบท้ายหนังสือรับต่ออายุขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน บริษัท ตรวจวัดสิ่งแวดล้อม จำกัด จำนวน ๑ แผ่น

ตามหนังสือที่อ้างถึง บริษัท ตรวจวัดสิ่งแวดล้อม จำกัด ขอต่ออายุหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน เลขทะเบียน ว-๓๐๑ สถานที่ตั้งเลขที่ ๕/๔๕ หมู่บ้าน บ้านกลางกรุง บิซทาวน์ ซอยศรีนครินทร์ ๔๖/๑ (ปราโมทย์) แขวงหนองบอน เขตประเวศ กรุงเทพมหานคร ต่อกรมโรงงานอุตสาหกรรม นั้น

กรมโรงงานอุตสาหกรรมพิจารณาแล้ว ให้บริษัท ตรวจวัดสิ่งแวดล้อม จำกัด ต่ออายุหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน โดยมีองค์ประกอบดังนี้

ก. ผู้ควบคุมดูแลห้องปฏิบัติการวิเคราะห์

ข.

ค.

หนังสือฉบับนี้จะหมดอายุในวันที่ ๓ มกราคม ๒๕๖๙ หากประสงค์จะต่ออายุหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน ให้ยื่นคำขอต่ออายุพร้อมเอกสารประกอบคำขอต่อกรมโรงงานอุตสาหกรรม ภายใน ๓๐ วัน ก่อนวันสิ้นอายุของหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน ทั้งนี้ สามารถยื่นคำขอผ่านระบบอิเล็กทรอนิกส์ได้ที่หน้าเว็บไซต์กรมโรงงานอุตสาหกรรม ตาม QR Code ท้ายหนังสือฉบับนี้

จึงเรียนมาเพื่อทราบ

CALIBRATION LABORATORY CO., LTD.
2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax. 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com
CLC Accredited ISO/IEC 17025
ilac-MRA
ANAB ANSI National Accreditation Board ACCREDITED CALIBRATION AND DIMENSIONAL MEASUREMENT ACDM-2814

MM-C20

REPORT OF CALIBRATION

FOR

NOMENCLATURE	:	DIGITAL THERMOMETER WITH PROBE
MANUFACTURER	:	LUTRON
MODEL / TYPE	:	MTM-380SD
SERIAL NO.	:	I.570147/N/A[LA-0013/LA-0013/A]
DATE OF CALIBRATION	:	09 April 2024

ENVIRONMENT CONDITIONS :

Temperature : (23 ± 2) °C Relative Humidity : (55 ± 10) % RH

PROCEDURE USED :

This instrument was calibrated under procedure No. **CLC-CPTH-06** based on **ASTM E 220-86** as calibration guidelines.
The calibration was performed by using Calibration Bath, Precision Thermometer and IPRT
which maintained by the Calibration Laboratory Co., Ltd.

REFERENCE STANDARD USED :

1. Calibration Bath, Kambic Model OB-22/2 ULT, OB-22/2 S/N. 17115653, 17115654.
2. Precision Thermometer, ASL Model F200-A-8 S/N. 014433/03.
3. IPRT, ASL Model T100-250-1D, T100-450-1D S/N. L0193A-1-1, L1123A-1-5.

TRACEABILITY :

1. The measurements are traceable to International System of Units (SI) , through Calibration Laboratory Co., Ltd.
Certificate No. Q23136342, Q23126517. Due Date 20 December 2024, 20 November 2024.
2. The measurements are traceable to International System of Units (SI) , through Thailand Institute of Scientific
and Technological Research (TISTR). Certificate No. PSL-T 0203/67, Due Date 07 December 2024.
3. The measurements are traceable to International System of Units (SI) , through National Institute of Metrology (Thailand).
Certificate No.TT-0136-23, TT-0132-23. Due Date 12 December 2024, 22 November 2024.

UNCERTAINTY :

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied
by the coverage factor $k = 2{,}00$ which for a normal distribution corresponds to a coverage probability of approximately 95 %.
It has been evaluated according to the "Evaluation of the Uncertainty of Measurement in Calibration (EA-4/02 M:2022)"

ข.17/2

CALIBRATION LABORATORY CO., LTD.
2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax. 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com
CLC Accredited ISO/IEC 17025
ilac-MRA
ANAB ANSI National Accreditation Board ACCREDITED CALIBRATION AND DIMENSIONAL MEASUREMENT ACDM-2814

CERTIFICATE OF CALIBRATION

FOR

NOMENCLATURE	:	DIGITAL THERMOMETER WITH PROBE
MANUFACTURER	:	LUTRON
MODEL / TYPE	:	MTM-380SD
SERIAL NO.	:	I.570147/N/A[LA-0013/LA-0013/A]
CLID. NO.	:	232204019
JOB CONTROL NO.	:	240408038373
CALIBRATION SERVICE	:	☑ IN-LABORATORY ☐ ON-SITE

CUSTOMER : ENVIRONMENTAL MEASUREMENTS CO., LTD.
5/45 BAAN KLANG KRUNG BIZ TOWN, SOI SRINAGARINDRA 46/1 (PRAMOTE),
NONG BON SUB-DISTRICT, PRAWET DISTRICT, BANGKOK 10250

DATE OF RECEIVED : 08 April 2024 DATE OF ISSUED : 10 April 2024

The report of calibration shall not be reproduced except in full without approval of the Calibration Laboratory Co., Ltd.

Calibrated By :

Approved By :

This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to the International System of Units (SI)

CALIBRATION LABORATORY CO., LTD.
2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com

MM-C20

CLC Accredited ISO/IEC 17025

ACCREDITED CALIBRATION AND DIMENSIONAL MEASUREMENT ACDM-2814

CERTIFICATE OF CALIBRATION

FOR

NOMENCLATURE	:	DO METER
MANUFACTURER	:	YSI
MODEL / TYPE	:	5000-230V/5010
SERIAL NO.	:	16D101626/19D100367[DOM-01]
CLID. NO.	:	272100329
JOB CONTROL NO.	:	240408038371
CALIBRATION SERVICE	:	☑ IN-LABORATORY ☐ ON-SITE

CUSTOMER : ENVIRONMENTAL MEASUREMENTS CO., LTD.
5/45 BAAN KLANG KRUNG BIZ TOWN, SOI SRINAGARINDRA 46/1 (PRAMOTE),
NONG BON SUB-DISTRICT, PRAWET DISTRICT, BANGKOK 10250

DATE OF RECEIVED : 08 April 2024 DATE OF ISSUED : 10 April 2024

The report of calibration shall not be reproduced except in full without approval of the Calibration Laboratory Co., Ltd.

Calibrated By :

Approved By :

This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to the International System of Units (SI)

Certificate No. Q24038371

F3-011-05/12-23

@clccalibration

9.17/3

CALIBRATION LABORATORY CO., LTD.
2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax. 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com

CLC Accredited ISO/IEC 17025

ACCREDITED CALIBRATION AND DIMENSIONAL MEASUREMENT ACDM-2814

CONDITION OF CALIBRATION ITEM : RECEIVED IN GOOD OPERATIONAL CONDITION

MEASUREMENT RESULTS : (X) without adjustment ( ) adjustment

The DUC Reading were recorded and the means value were reported of five times measurement in the table below.

CALIBRATION DATA

CORRECTION OF TEMPERATURE : T1 [THERMOCOUPLE TYPE K]

Immersion depth (mm)	Actual Temperature (°C)	DUC Reading (°C)	Correction (°C)	Uncertainty ± (°C)
200	4.00	4.2	-0.20	0.52
	20.01	20.3	-0.29	
	95.04	95.6	-0.56	
	104.02	104.9	-0.88	
	180.03	181.4	-1.37	

Note. The Scope of Accredited ANAB Certificate No. ACDM-2814 Version 012 Page 56 of 67

This report is valid for the above stated instrument/s only.

End of Certificate

Certificate No. Q24038373

F3-011-05/12-23

@clccalibration

CALIBRATION LABORATORY CO., LTD.
2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com
CLC Accredited ISO/IEC 17025
ACCREDITED CALIBRATION AND DIMENSIONAL MEASUREMENT ACDM-2814

CONDITION OF CALIBRATION ITEM : RECEIVED IN GOOD OPERATIONAL CONDITION

MEASUREMENT RESULTS : (X) without adjustment ( ) adjustment

The table in the following gives the calibration results and associated measurement uncertainties of Do Meter.

CALIBRATION DATA

CORRECTION OF DO METER @ 20°C

Nominal Value (mg/L)	DUC Reading (mg/L)	Correction (mg/L)	Uncertainty (mg/L)
7.78	7.80	-0.02	± 0.38

Note. The Scope of Accredited ANAB Certificate No. ACDM-2814 Version 012 Page 5 of 67

This report is valid for the above stated instrument/s only.

End of Certificate

CALIBRATION LABORATORY CO., LTD.
2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com
CLC Accredited ISO/IEC 17025
ACCREDITED CALIBRATION AND DIMENSIONAL MEASUREMENT ACDM-2814

REPORT OF CALIBRATION

FOR

NOMENCLATURE	:	**DO METER**
MANUFACTURER	:	**YSI**
MODEL / TYPE	:	**5000-230V/5010**
SERIAL NO.	:	**16D101626/19D100367[DOM-01]**
DATE OF CALIBRATION	:	**09 April 2024**

ENVIRONMENT CONDITIONS :

Temperature : (25 ± 2.5) °C **Relative Humidity :** (50 ± 15) %RH

PROCEDURE USED :

This instrument was calibrated under procedure No. **CLC-CPCH-06.** The calibration was performed by direct measurement with Certified Reference Material (CRM).

REFERENCE STANDARD USED :

Dissolved Oxygen, Sigma-Alorich Product ID QC3077-500ML .

TRACEABILITY :

The measurements are traceable to International System of Units (SI) , through Merck Co., Ltd.
Lot LRAD3840 , Due Date October 2024.

UNCERTAINTY :

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor $k = 2{,}00$ which for a normal distribution corresponds to a coverage probability of approximately 95 %. It has been evaluated according to the "Evaluation of the Uncertainty of Measurement in Calibration (EA-4/02 M:2022)"

CALIBRATION LABORATORY CO., LTD.
2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax. 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com

MM-C20

CLC Accredited ISO/IEC 17025

ilac-MRA

ANAB ANSI National Accreditation Board ACCREDITED CALIBRATION AND DIMENSIONAL MEASUREMENT ACDM-2814

REPORT OF CALIBRATION

FOR

NOMENCLATURE	:	DIGITAL THERMOHYGRO METER
MANUFACTURER	:	DIGICON
MODEL / TYPE	:	TH-02A
SERIAL NO.	:	1919E0284980[DTH-02]
DATE OF CALIBRATION	:	10 April 2024

ENVIRONMENT CONDITIONS :

Temperature : (23 ± 2) °C **Relative Humidity :** (55 ± 10) %RH

PROCEDURE USED :

This instrument was calibrated under procedure No. **CLC-CPTH-11.** The calibration was performed by using Chilled Mirror Hygrometer which maintained by the Calibration Laboratory Co., Ltd.

REFERENCE STANDARD USED :

Chilled Mirror Hygrometer, Edgetech Model Dew Master S/N. 44602.

Temperature & Humidity Chamber, PGC Model 9141-5116 S/N. 1304261.

TRACEABILITY :

The measurements are traceable to International System of Units (SI) , through Thunder Scientific Corporation.

Certificate No. 21594, Due Date 06 July 2024.

UNCERTAINTY :

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k = 2,00 which for a normal distribution corresponds to a coverage probability of approximately 95 %. It has been evaluated according to the "Evaluation of the Uncertainty of Measurement in Calibration (EA-4/02 M:2022)"

@clccalibration

9.17/5

CALIBRATION LABORATORY CO., LTD.
2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax. 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com

CLC Accredited ISO/IEC 17025

ilac-MRA

ANAB ANSI National Accreditation Board ACCREDITED CALIBRATION AND DIMENSIONAL MEASUREMENT ACDM-2814

CERTIFICATE OF CALIBRATION

FOR

NOMENCLATURE	:	DIGITAL THERMOHYGRO METER
MANUFACTURER	:	DIGICON
MODEL / TYPE	:	TH-02A
SERIAL NO.	:	1919E0284980[DTH-02]
CLID. NO.	:	232100201
JOB CONTROL NO.	:	240408038370
CALIBRATION SERVICE	:	☑ IN-LABORATORY ☐ ON-SITE

CUSTOMER : ENVIRONMENTAL MEASUREMENTS CO., LTD.
5/45 BAAN KLANG KRUNG BIZ TOWN, SOI SRINAGARINDRA 46/1 (PRAMOTE),
NONG BON SUB-DISTRICT, PRAWET DISTRICT, BANGKOK 10250

DATE OF RECEIVED : 08 April 2024 DATE OF ISSUED : 17 April 2024

The report of calibration shall not be reproduced except in full without approval of the Calibration Laboratory Co., Ltd.

Calibrated By :

Approved By :

This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to the International System of Units (SI)

@clccalibration

CALIBRATION LABORATORY CO., LTD.
2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax. 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com
CLC Accredited ISO/IEC 17025
ACCREDITED CALIBRATION AND DIMENSIONAL MEASUREMENT ACDM-2814

MM-C20

CERTIFICATE OF CALIBRATION

FOR

NOMENCLATURE	:	DIGITAL THERMOHYGRO METER
MANUFACTURER	:	DIGICON
MODEL / TYPE	:	TH-02A
SERIAL NO.	:	1919E0284991[DTH-01]
CLID. NO.	:	232100200
JOB CONTROL NO.	:	240408038369
CALIBRATION SERVICE	:	☑ IN-LABORATORY ☐ ON-SITE

CUSTOMER : ENVIRONMENTAL MEASUREMENTS CO., LTD.
5/45 BAAN KLANG KRUNG BIZ TOWN, SOI SRINAGARINDRA 46/1 (PRAMOTE),
NONG BON SUB-DISTRICT, PRAWET DISTRICT, BANGKOK 10250

DATE OF RECEIVED : 08 April 2024 DATE OF ISSUED : 17 April 2024

The report of calibration shall not be reproduced except in full without approval of the Calibration Laboratory Co., Ltd.

Calibrated By :

Approved By :

This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to the International System of Units (SI)

9.17/6

CALIBRATION LABORATORY CO., LTD.
2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax. 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com
CLC Accredited ISO/IEC 17025
ACCREDITED CALIBRATION AND DIMENSIONAL MEASUREMENT ACDM-2814

CONDITION OF CALIBRATION ITEM : RECEIVED IN GOOD OPERATIONAL CONDITION

MEASUREMENT RESULTS : (X) without adjustment ( ) adjustment

The table in the following gives the calibration results and associated measurement uncertainties of the measuring digital thermohygro meter.

CALIBRATION DATA

1. CORRECTION OF TEMPERATURE

Test point (°C)	Actual Temperature (°C)	DUC Reading (°C)	Correction (°C)	Uncertainty ±(°C)
20.0	20.00	19.7	+0.30	0.27
25.0	25.00	24.7	+0.30	
30.0	30.00	29.6	+0.40	

2. CORRECTION OF HUMIDITY

STD Temperature (°C)	STD Reading (%RH)	DUC Reading (%RH)	Correction (%RH)	Uncertainty ± (%RH)
25	40.0	33	+7.0	0.8
25	60.0	53	+7.0	0.9

Note. The Scope of Accredited ANAB Certificate No. ACDM-2814 Version 012 Page 59 of 67

This report is valid for the above stated instrument/s only.

End of Certificate

CONDITION OF CALIBRATION ITEM : RECEIVED IN GOOD OPERATIONAL CONDITION

MEASUREMENT RESULTS : (X) without adjustment ( ) adjustment

The table in the following gives the calibration results and associated measurement uncertainties of the measuring digital thermohygro meter.

CALIBRATION DATA

1. CORRECTION OF TEMPERATURE

Test point (°C)	Actual Temperature (°C)	DUC Reading (°C)	Correction (°C)	Uncertainty ±(°C)
20.0	20.00	19.6	+0.40	0.27
25.0	25.00	24.6	+0.40	
30.0	30.00	29.5	+0.50	

2. CORRECTION OF HUMIDITY

STD Temperature (°C)	STD Reading (%RH)	DUC Reading (%RH)	Correction (%RH)	Uncertainty ± (%RH)
25	40.0	32	+8.0	0.8
25	60.0	52	+8.0	0.9

Note. The Scope of Accredited ANAB Certificate No. ACDM-2814 Version 012 Page 59 of 67

This report is valid for the above stated instrument/s only.

End of Certificate

CALIBRATION LABORATORY CO., LTD.
2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax. 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com
CLC Accredited ISO/IEC 17025
ACCREDITED CALIBRATION AND DIMENSIONAL MEASUREMENT ACDM-2814

REPORT OF CALIBRATION

FOR

NOMENCLATURE	:	**DIGITAL THERMOHYGRO METER**
MANUFACTURER	:	**DIGICON**
MODEL / TYPE	:	**TH-02A**
SERIAL NO.	:	**1919E0284991[DTH-01]**
DATE OF CALIBRATION	:	**10 April 2024**

ENVIRONMENT CONDITIONS :

Temperature : **(23 ± 2) °C** **Relative Humidity :** **(55 ± 10) %RH**

PROCEDURE USED :

This instrument was calibrated under procedure No. **CLC-CPTH-11.** The calibration was performed by using Chilled Mirror Hygrometer which maintained by the Calibration Laboratory Co., Ltd.

REFERENCE STANDARD USED :

Chilled Mirror Hygrometer, Edgetech Model Dew Master S/N. 44602.

Temperature & Humidity Chamber, PGC Model 9141-5116 S/N. 1304261.

TRACEABILITY :

The measurements are traceable to International System of Units (SI) , through Thunder Scientific Corporation.

Certificate No. 21594, Due Date 06 July 2024.

UNCERTAINTY :

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor $k = 2{,}00$ which for a normal distribution corresponds to a coverage probability of approximately 95 %.

It has been evaluated according to the "Evaluation of the Uncertainty of Measurement in Calibration (EA-4/02 M:2022)"

CALIBRATION LABORATORY CO., LTD.
2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com
CLC Accredited ISO/IEC 17025
ilac-MRA
THAILAND
NSC-TISI-TIS 17025
CALIBRATION 0059
CLC

REPORT OF CALIBRATION

FOR

NOMENCLATURE	:	WATER BATH
MANUFACTURER	:	M-LAB
MODEL / TYPE	:	WBN 15
SERIAL NO.	:	0335[LA-007]
LOCATION SITE	:	LABORATORY-HOT ZONE
DATE OF CALIBRATION	:	04 April 2024

ENVIRONMENT CONDITIONS :

Temperature : 24 °C to 25 °C **Relative Humidity : 50% to 52%**

PROCEDURE USED :

This instrument was calibrated under procedure No. **WI-305-135** based on **ASTM E 715-80:2016** as calibration guidelines.

The calibration was performed by using Hydra Series II which maintained by the Calibration Laboratory Co., Ltd.

REFERENCE STANDARD USED :

Hydra Series II, Fluke Model 2635A S/N. 7107303.

TRACEABILITY :

The measurements are traceable to International System of Units (SI) , through Calibration Laboratory Co., Ltd.

Certificate No. Q24026699, Due Date 13 September 2024.

UNCERTAINTY :

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor $k = 2{,}00$ which for a normal distribution corresponds to a coverage probability of approximately 95 %.

It has been evaluated according to the "Evaluation of the Uncertainty of Measurement in Calibration (EA-4/02 M:2022)"

@clccalibration

CALIBRATION LABORATORY CO., LTD.
2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com
CLC Accredited ISO/IEC 17025
ilac-MRA
THAILAND
NSC-TISI-TIS 17025
CALIBRATION 0059
CLC

CERTIFICATE OF CALIBRATION

FOR

NOMENCLATURE	:	WATER BATH
MANUFACTURER	:	M-LAB
MODEL / TYPE	:	WBN 15
SERIAL NO.	:	0335[LA-007]
CLID. NO.	:	332300657
JOB CONTROL NO.	:	240307024795
CALIBRATION SERVICE	:	☐ IN-LABORATORY ☑ ON-SITE

CUSTOMER : ENVIRONMENTAL MEASUREMENTS CO., LTD.
5/45 BAAN KLANG KRUNG BIZ TOWN, SOI SRINAGARINDRA 46/1 (PRAMOTE),
NONG BON SUB-DISTRICT, PRAWET DISTRICT, BANGKOK 10250

DATE OF RECEIVED : 07 March 2024 DATE OF ISSUED : 06 April 2024

The report of calibration shall not be reproduced except in full without approval of the Calibration Laboratory Co., Ltd.

Calibrated By :

Approved By :

06 April 2024

This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to the International System of Units (SI)

@clccalibration

CALIBRATION DATA

2. TEMPERATURE DISTRIBUTION

Test Point (°C)	DUC Reading (°C)	STD Reading (°C)					Uncertainty ±(°C)
		Probe No. 1	Probe No. 2	Probe No. 3	Probe No. 4	Probe No. 5	
85.0	85.0	84.37	84.87	84.67	84.86	84.71	0.60

Technical Note : W = 35 cm, D = 30 cm, H = 15 cm.

The Scope of Accredited TISI Certificate No. 23-LB0092 Issue 02 Page 128 of 138

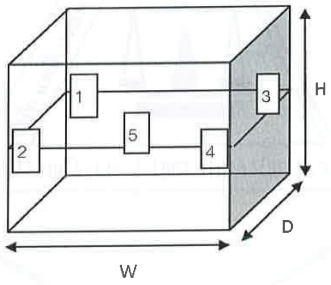

This report is valid for the above stated instrument/s only.

End of Certificate

CALIBRATION LABORATORY CO., LTD.
2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com
CLC Accredited ISO/IEC 17025
NSC-TISI-TIS 17025 CALIBRATION 0059 CLC

CONDITION OF CALIBRATION ITEM : RECEIVED IN GOOD OPERATIONAL CONDITION

MEASUREMENT RESULTS : (X) without adjustment ( ) adjustment

The table in the following gives the calibration results and associated measurement uncertainties of the measuring water bath.

CALIBRATION DATA

1. WATER BATH PERFORMANCE

Test Point (°C)	DUC Reading (°C)	Uniformity (°C)	Stability (°C)
85.0	85.0	0.48	0.17

CALIBRATION LABORATORY CO., LTD.
2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com
CLC Accredited ISO/IEC 17025
NSC-TISI-TIS 17025 CALIBRATION 0059 CLC

REPORT OF CALIBRATION

FOR

NOMENCLATURE	:	WATER BATH
MANUFACTURER	:	MEMMERT
MODEL / TYPE	:	WNB14
SERIAL NO.	:	L418.0758[LA-004]
LOCATION SITE	:	LABORATORY-HOT ZONE
DATE OF CALIBRATION	:	04 April 2024

ENVIRONMENT CONDITIONS :

Temperature : 24 °C to 25 °C **Relative Humidity : 50% to 52%**

PROCEDURE USED :

This instrument was calibrated under procedure No. **WI-305-135** based on **ASTM E 715-80:2016** as calibration guidelines.

The calibration was performed by using Hydra Series II which maintained by the Calibration Laboratory Co., Ltd.

REFERENCE STANDARD USED :

Hydra Series II, Fluke Model 2635A S/N. 7107303.

TRACEABILITY :

The measurements are traceable to International System of Units (SI) , through Calibration Laboratory Co., Ltd.

Certificate No. Q24026699, Due Date 13 September 2024.

UNCERTAINTY :

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor $k = 2{,}00$ which for a normal distribution corresponds to a coverage probability of approximately 95 %.

It has been evaluated according to the "Evaluation of the Uncertainty of Measurement in Calibration (EA-4/02 M:2022)"

CALIBRATION LABORATORY CO., LTD.
2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com
CLC Accredited ISO/IEC 17025
NSC-TISI-TIS 17025 CALIBRATION 0059 CLC

CERTIFICATE OF CALIBRATION

FOR

NOMENCLATURE	:	WATER BATH
MANUFACTURER	:	MEMMERT
MODEL / TYPE	:	WNB14
SERIAL NO.	:	L418.0758[LA-004]
CLID. NO.	:	332100157
JOB CONTROL NO.	:	240307024794
CALIBRATION SERVICE	:	☐ IN-LABORATORY ☑ ON-SITE

CUSTOMER : ENVIRONMENTAL MEASUREMENTS CO., LTD.
5/45 BAAN KLANG KRUNG BIZ TOWN, SOI SRINAGARINDRA 46/1 (PRAMOTE),
NONG BON SUB-DISTRICT, PRAWET DISTRICT, BANGKOK 10250

DATE OF RECEIVED : 07 March 2024 **DATE OF ISSUED : 06 April 2024**

The report of calibration shall not be reproduced except in full without approval of the Calibration Laboratory Co., Ltd.

Calibrated By :

Approved By :

This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to the International System of Units (SI)

CALIBRATION DATA

2. TEMPERATURE DISTRIBUTION

Test Point (°C)	DUC Reading (°C)	STD Reading (°C)					Uncertainty ±(°C)
		Probe No. 1	Probe No. 2	Probe No. 3	Probe No. 4	Probe No. 5	
95.0	95.0	96.62	96.74	96.93	96.68	96.66	0.65

Technical Note : W = 35 cm, D = 29 cm, H = 14 cm.

The Scope of Accredited TISI Certificate No. 23-LB0092 Issue 02 Page 128 of 138

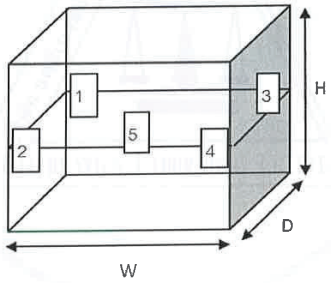

This report is valid for the above stated instrument/s only.

End of Certificate

CALIBRATION LABORATORY CO., LTD.
2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com
CLC Accredited ISO/IEC 17025
NSC-TISI-TIS 17025 CALIBRATION 0059 CLC

CONDITION OF CALIBRATION ITEM : RECEIVED IN GOOD OPERATIONAL CONDITION

MEASUREMENT RESULTS : (X) without adjustment ( ) adjustment

The table in the following gives the calibration results and associated measurement uncertainties of the measuring water bath.

CALIBRATION DATA

1. WATER BATH PERFORMANCE

Test Point (°C)	DUC Reading (°C)	Uniformity (°C)	Stability (°C)
95.0	95.0	0.50	0.21

CALIBRATION LABORATORY CO., LTD.
2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com
CLC Accredited ISO/IEC 17025
NSC-TISI-TIS 17025 CALIBRATION 0059 CLC

REPORT OF CALIBRATION

FOR

NOMENCLATURE	:	REFRIGERATOR
MANUFACTURER	:	MEDICOOL
MODEL / TYPE	:	BB-117
SERIAL NO.	:	BB117-190725001[LA-003]
LOCATION SITE	:	LABORATORY
DATE OF CALIBRATION	:	04 April 2024

ENVIRONMENT CONDITIONS :

Temperature : 24 °C to 25 °C **Relative Humidity : 50 % to 52 %**

PROCEDURE USED :

This instrument was calibrated under procedure No. **WI-305-165** based on **TLAS G-20-1/02-08** as calibration guidelines.

The calibration was performed by using Hydra Data Logger which maintained by the Calibration Laboratory Co., Ltd.

REFERENCE STANDARD USED :

Hydra Data Logger, Fluke Model 2620 S/N. 5592550.

TRACEABILITY :

The measurements are traceable to International System of Units (SI) , through Calibration Laboratory Co., Ltd.

Certificate No. Q23065868, Due Date 22 June 2024.

UNCERTAINTY :

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor complies with the table which for a normal distribution corresponds to a coverage probability of approximately 95 %.

It has been evaluated according to the "Evaluation of the Uncertainty of Measurement in Calibration (EA-4/02 M:2022)"

CALIBRATION LABORATORY CO., LTD.
2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com
CLC Accredited ISO/IEC 17025
NSC-TISI-TIS 17025 CALIBRATION 0059 CLC

CERTIFICATE OF CALIBRATION

FOR

NOMENCLATURE	:	REFRIGERATOR
MANUFACTURER	:	MEDICOOL
MODEL / TYPE	:	BB-117
SERIAL NO.	:	BB117-190725001[LA-003]
CLID. NO.	:	332100156
JOB CONTROL NO.	:	240307024793
CALIBRATION SERVICE	:	☐ IN-LABORATORY ☑ ON-SITE

CUSTOMER : ENVIRONMENTAL MEASUREMENTS CO., LTD.
5/45 BAAN KLANG KRUNG BIZ TOWN, SOI SRINAGARINDRA 46/1 (PRAMOTE),
NONG BON SUB-DISTRICT, PRAWET DISTRICT, BANGKOK 10250

DATE OF RECEIVED : 07 March 2024 **DATE OF ISSUED : 06 April 2024**

The report of calibration shall not be reproduced except in full without approval of the Calibration Laboratory Co., Ltd.

Calibrated By :

Approved By :

This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to the International System of Units (SI)

CALIBRATION DATA

2. TEMPERATURE DISTRIBUTION

DUC		Measured Temperature (°C)@Probe No.9 is Ref.									Uncertainty ±(°C)	Coverage factor *k*
Setting (°C)	Indicating (°C)	1	2	3	4	5	6	7	8	9		
4.0	4.0	3.22	3.93	3.21	3.93	3.52	3.29	3.02	3.18	3.31	1.40	2,00

Technical Note : W = 50 cm, D = 50 cm, H = 120 cm.

The Scope of Accredited TISI Certificate No. 23-LB0092 Issue 02 Page 129 of 138

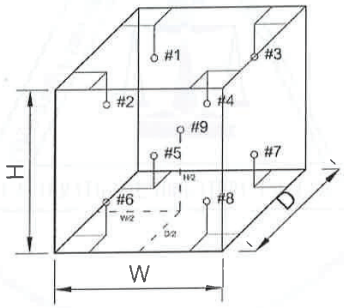

This report is valid for the above stated instrument/s only.

End of Certificate

CALIBRATION LABORATORY CO., LTD.
2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com
CLC Accredited ISO/IEC 17025
NSC-TISI-TIS 17025 CALIBRATION 0059 CLC

CONDITION OF CALIBRATION ITEM : RECEIVED IN GOOD OPERATIONAL CONDITION

MEASUREMENT RESULTS : (X) without adjustment ( ) adjustment

The table in the following gives the calibration results and associated measurement uncertainties of the measuring refrigerator.

CALIBRATION DATA

1. REFRIGERATOR PERFORMANCE

DUC		Measured Uniformity (°C)	Measured Stability (°C)	Measured Overall Variation (°C)
Setting (°C)	Indicating (°C)			
4.0	4.0	0.82	1.14	2.49

CALIBRATION LABORATORY CO., LTD.
2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com
CLC Accredited ISO/IEC 17025
ilac-MRA
NSC-TISI-TIS 17025 CALIBRATION 0059 CLC

REPORT OF CALIBRATION

FOR

NOMENCLATURE	:	INCUBATOR
MANUFACTURER	:	ACCUPLUS
MODEL / TYPE	:	SMART i250
SERIAL NO.	:	2059-0718-0010[LA-002]
LOCATION SITE	:	LABORATORY
DATE OF CALIBRATION	:	04 April 2024

ENVIRONMENT CONDITIONS :

Temperature : 24 °C to 25 °C **Relative Humidity : 50 % to 52 %**

PROCEDURE USED :

This instrument was calibrated under procedure No. **WI-305-165** based on **TLAS G-20-1/02-08** as calibration guidelines.

The calibration was performed by using Hydra Data Logger which maintained by the Calibration Laboratory Co., Ltd.

REFERENCE STANDARD USED :

Hydra Data Logger, Fluke Model 2620 S/N. 5592550.

TRACEABILITY :

The measurements are traceable to International System of Units (SI) , through Calibration Laboratory Co., Ltd.

Certificate No. Q23065868, Due Date 22 June 2024.

UNCERTAINTY :

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor complies with the table which for a normal distribution corresponds to a coverage probability of approximately 95 %.

It has been evaluated according to the "Evaluation of the Uncertainty of Measurement in Calibration (EA-4/02 M:2022)"

CALIBRATION LABORATORY CO., LTD.
2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com
CLC Accredited ISO/IEC 17025
ilac-MRA
NSC-TISI-TIS 17025 CALIBRATION 0059 CLC

CERTIFICATE OF CALIBRATION

FOR

NOMENCLATURE	:	INCUBATOR
MANUFACTURER	:	ACCUPLUS
MODEL / TYPE	:	SMART i250
SERIAL NO.	:	2059-0718-0010[LA-002]
CLID. NO.	:	332100155
JOB CONTROL NO.	:	240307024792
CALIBRATION SERVICE	:	☐ IN-LABORATORY ☑ ON-SITE

CUSTOMER : ENVIRONMENTAL MEASUREMENTS CO., LTD.
5/45 BAAN KLANG KRUNG BIZ TOWN, SOI SRINAGARINDRA 46/1 (PRAMOTE),
NONG BON SUB-DISTRICT, PRAWET DISTRICT, BANGKOK 10250

DATE OF RECEIVED : 07 March 2024 **DATE OF ISSUED : 06 April 2024**

The report of calibration shall not be reproduced except in full without approval of the Calibration Laboratory Co., Ltd.

Calibrated By :

Approved By :

This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to the International System of Units (SI)

CALIBRATION DATA

2. TEMPERATURE DISTRIBUTION

DUC		Measured Temperature (°C)@Probe No.9 is Ref.									Uncertainty ±(°C)	Coverage factor *k*
Setting (°C)	Indicating (°C)	1	2	3	4	5	6	7	8	9		
20.0	20.0	20.58	20.70	20.70	20.46	20.54	20.53	20.53	20.36	20.39	0.68	2,00

Technical Note : W = 50 cm, D = 48 cm, H = 110 cm.

The Scope of Accredited TISI Certificate No. 23-LB0092 Issue 02 Page 129 of 138

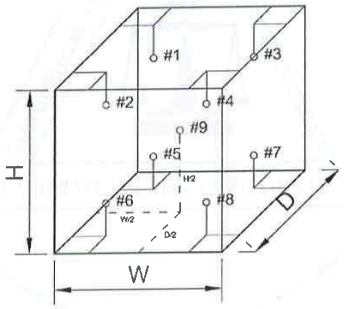

This report is valid for the above stated instrument/s only.

End of Certificate

CALIBRATION LABORATORY CO., LTD.
2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com
CLC Accredited ISO/IEC 17025
ilac-MRA
NSC-TISI-TIS 17025
CALIBRATION 0059
CLC

CONDITION OF CALIBRATION ITEM : RECEIVED IN GOOD OPERATIONAL CONDITION

MEASUREMENT RESULTS : (X) without adjustment ( ) adjustment

The table in the following gives the calibration results and associated measurement uncertainties of the measuring incubator.

CALIBRATION DATA

1. INCUBATOR PERFORMANCE

DUC		Measured Uniformity (°C)	Measured Stability (°C)	Measured Overall Variation (°C)
Setting (°C)	Indicating (°C)			
20.0	20.0	0.52	0.46	1.06

CALIBRATION LABORATORY CO., LTD.
2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com
CLC Accredited ISO/IEC 17025
ilac-MRA
ANAB ACCREDITED CALIBRATION AND DIMENSIONAL MEASUREMENT ACDM-2814

REPORT OF CALIBRATION

FOR

NOMENCLATURE	:	HOT AIR OVEN
MANUFACTURER	:	MEMMERT
MODEL / TYPE	:	UF110
SERIAL NO.	:	B422.0026[LA-0012]
LOCATION SITE	:	LABORATORY-HOT ZONE
DATE OF CALIBRATION	:	04 April 2024

ENVIRONMENT CONDITIONS :

Temperature : 24 °C to 25 °C Relative Humidity : 50% to 52 %

PROCEDURE USED :

This instrument was calibrated under procedure No. **CLC-CPTH-07** based on **TLAS G-20** as calibration guidelines.

The calibration was performed by using Hydra Data Logger which maintained by the Calibration Laboratory Co., Ltd.

REFERENCE STANDARD USED :

Hydra Data Logger, Fluke Model 2620 S/N. 5592550.

TRACEABILITY :

The measurements are traceable to International System of Units (SI) , through Calibration Laboratory Co., Ltd.

Certificate No. Q23065868, Due Date 22 June 2024.

UNCERTAINTY :

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor complies with the table which for a normal distribution corresponds to a coverage probability of approximately 95 %.

It has been evaluated according to the "Evaluation of the Uncertainty of Measurement in Calibration (EA-4/02 M:2022)"

CALIBRATION LABORATORY CO., LTD.
2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com
CLC Accredited ISO/IEC 17025
ilac-MRA
ANAB ACCREDITED CALIBRATION AND DIMENSIONAL MEASUREMENT ACDM-2814

CERTIFICATE OF CALIBRATION

FOR

NOMENCLATURE	:	HOT AIR OVEN
MANUFACTURER	:	MEMMERT
MODEL / TYPE	:	UF110
SERIAL NO.	:	B422.0026[LA-0012]
CLID. NO.	:	332202464
JOB CONTROL NO.	:	240307024791
CALIBRATION SERVICE	:	☐ IN-LABORATORY ☑ ON-SITE

CUSTOMER : ENVIRONMENTAL MEASUREMENTS CO., LTD.
5/45 BAAN KLANG KRUNG BIZ TOWN, SOI SRINAGARINDRA 46/1 (PRAMOTE),
NONG BON SUB-DISTRICT, PRAWET DISTRICT, BANGKOK 10250

DATE OF RECEIVED : 07 March 2024 DATE OF ISSUED : 06 April 2024

The report of calibration shall not be reproduced except in full without approval of the Calibration Laboratory Co., Ltd.

Calibrated By :

Approved By :

This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to the International System of Units (SI)

CALIBRATION DATA

2. TEMPERATURE DISTRIBUTION

DUC		Measured Temperature (°C)@Probe No.9 is Ref.									Uncertainty ±(°C)	Coverage factor *k*
Setting (° C)	Indicating (° C)	1	2	3	4	5	6	7	8	9		
104.0	104.0	103.11	104.12	103.56	103.79	103.72	103.88	103.57	104.18	103.88	0.45	2,00
180.0	180.0	178.33	180.32	178.77	179.54	179.26	179.74	179.19	180.15	179.58	0.55	2,00

Technical Note : W = 56 cm, D = 40 cm, H = 48 cm.

Note. The Scope of Accredited ANAB Certificate No. ACDM-2814 Version 012 Page 58 of 67

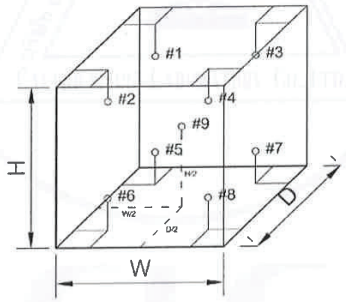

This report is valid for the above stated instrument/s only.

End of Certificate

CLC Accredited ISO/IEC 17025

CALIBRATION LABORATORY CO., LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230

Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com

ilac-MRA

ANAB ANSI National Accreditation Board ACCREDITED CALIBRATION AND DIMENSIONAL MEASUREMENT ACDM-2814

CONDITION OF CALIBRATION ITEM : RECEIVED IN GOOD OPERATIONAL CONDITION

MEASUREMENT RESULTS : (X) without adjustment ( ) adjustment

The table in the following gives the calibration results and associated measurement uncertainties of the measuring hot air oven.

CALIBRATION DATA

1. HOT AIR OVEN PERFORMANCE

DUC		Measured Uniformity (°C)	Measured Stability (°C)	Measured Overall Variation (°C)
Setting (°C)	Indicating (°C)			
104.0	104.0	0.81	0.07	1.20
180.0	180.0	1.35	0.19	2.17

CALIBRATION LABORATORY CO., LTD.
2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com
CLC Accredited ISO/IEC 17025
NSC-TISI-TIS 17025 CALIBRATION 0059 CLC

MM-C20

REPORT OF CALIBRATION

FOR

NOMENCLATURE	:	BALANCE
MANUFACTURER	:	METTLER TOLEDO
MODEL / TYPE	:	MS204TS/00
SERIAL NO.	:	B935191252[LA-002]
LOCATION SITE	:	LABORATORY - BALANCE ROOM
DATE OF CALIBRATION	:	04 April 2024

ENVIRONMENT CONDITIONS :

Temperature : 24 °C to 25 °C Relative Humidity : 50 % to 51 %

PROCEDURE USED :

This instrument was calibrated under procedure No. **WI-305-46** based on **EURAMET cg-18 Version 4.0 (11/2015).**

The calibration was performed by Comparison with Weight Set which maintained by the Calibration Laboratory Co., Ltd.

REFERENCE STANDARD USED :

1. Weight Set, Phoenix Class E2 S/N. WBS-SET-E2-01.
2. Weight, Sartorius Class E2 S/N. 44329129, 43529037, 44329167, 43529293.

TRACEABILITY :

1. The measurements are traceable to International System of Units (SI), through National Institute of Metrology (Thailand). Certificate No. MM-0123-22, Due Date 22 August 2024.
2. The measurements are traceable to International System of Units (SI) , through Sartorius Lab Instruments GmbH & Co. KG. Certificate No. M141607, M141608, M141609, M141611. Due Date 15 September 2025.

UNCERTAINTY :

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor complies with the table which for a normal distribution corresponds to a coverage probability of approximately 95%. It has been evaluated according to the "Evaluation of the Uncertainty of Measurement in Calibration (EA-4/02 M:2022)"

CALIBRATION LABORATORY CO., LTD.
2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com
CLC Accredited ISO/IEC 17025
NSC-TISI-TIS 17025 CALIBRATION 0059 CLC

CERTIFICATE OF CALIBRATION

FOR

NOMENCLATURE	:	BALANCE
MANUFACTURER	:	METTLER TOLEDO
MODEL / TYPE	:	MS204TS/00
SERIAL NO.	:	B935191252[LA-002]
CLID. NO.	:	362200356
JOB CONTROL NO.	:	240307024790
CALIBRATION SERVICE	:	☐ IN-LABORATORY ☑ ON-SITE

CUSTOMER : ENVIRONMENTAL MEASUREMENTS CO., LTD.
5/45 BAAN KLANG KRUNG BIZ TOWN, SOI SRINAGARINDRA 46/1 (PRAMOTE),
NONG BON SUB-DISTRICT, PRAWET DISTRICT, BANGKOK 10250

DATE OF RECEIVED : 07 March 2024 DATE OF ISSUED : 08 April 2024

The report of calibration shall not be reproduced except in full without approval of the Calibration Laboratory Co., Ltd.

Calibrated By :

Approved By :

08 April 2024

This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to the International System of Units (SI)

CALIBRATION LABORATORY CO., LTD.
2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com
CLC Accredited ISO/IEC 17025
NSC-TISI-TIS 17025 CALIBRATION 0059 CLC

MM-C20

CERTIFICATE OF CALIBRATION

FOR

NOMENCLATURE	:	BALANCE
MANUFACTURER	:	SHIMADZU
MODEL / TYPE	:	AP225WD
SERIAL NO.	:	D316300692[LA-001]
CLID. NO.	:	362100172
JOB CONTROL NO.	:	240307024789
CALIBRATION SERVICE	:	☐ IN-LABORATORY ☑ ON-SITE

CUSTOMER : ENVIRONMENTAL MEASUREMENTS CO., LTD.
5/45 BAAN KLANG KRUNG BIZ TOWN, SOI SRINAGARINDRA 46/1 (PRAMOTE),
NONG BON SUB-DISTRICT, PRAWET DISTRICT, BANGKOK 10250

DATE OF RECEIVED : 07 March 2024 DATE OF ISSUED : 05 April 2024

The report of calibration shall not be reproduced except in full without approval of the Calibration Laboratory Co., Ltd.

Calibrated By :

Approved By :

This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to the International System of Units (SI)

Certificate No. Q24024789

F3-011-05/12-23

@clccalibration

9.17/19

CALIBRATION LABORATORY CO., LTD.
2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com
CLC Accredited ISO/IEC 17025
NSC-TISI-TIS 17025 CALIBRATION 0059 CLC

CONDITION OF CALIBRATION ITEM : RECEIVED IN GOOD OPERATIONAL CONDITION

MEASUREMENT RESULTS : (X) without adjustment ( ) adjustment

CALIBRATION DATA

1. Error of indications

Nominal Test Value (g)	Conventional mass (g)	Display Value (g)	Error of Balance (g)	Uncertainty ± (mg)	Coverage factor *k*
Unload	0.0000	0.0000	0.0000	0.07	2,00
0.1000	0.1000	0.0999	-0.0001	0.11	2,00
0.5000	0.5000	0.5000	0.0000	0.11	2,00
1.0000	1.0000	1.0000	0.0000	0.11	2,00
2.0000	2.0000	2.0000	0.0000	0.11	2,00
5.0000	5.0000	4.9999	-0.0001	0.11	2,00
10.0000	10.0000	9.9999	-0.0001	0.11	2,00

2. Repeatability of indications

Nominal Test Value (g)	Standard Deviation of Reading (g)
200.0000	0.00005

3. Effect of eccentric application of a load on the indication

☐ 

☑ 

Nominal Test Value (g)	Display Value (g)					Maximum Difference of Center Value (g)
	Position 1	Position 2	Position 3	Position 4	Position 5	
100.0000	100.0000	100.0001	100.0001	99.9999	100.0001	0.0001

Note. The Scope of Accredited TISI Certificate No. 23-LB0092 Issue 02 Page 116 of 138

This report is valid for the above stated instrument/s only.

End of Certificate

Certificate No. Q24024790

F3-011-05/12-23

@clccalibration

CALIBRATION LABORATORY CO., LTD.
2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com
CLC Accredited ISO/IEC 17025
NSC-TISI-TIS 17025 CALIBRATION 0059 CLC

CONDITION OF CALIBRATION ITEM : RECEIVED IN GOOD OPERATIONAL CONDITION

MEASUREMENT RESULTS : (X) without adjustment ( ) adjustment

CALIBRATION DATA

1. Error of indications

Nominal Test Value (g)	Conventional mass (g)	Display Value (g)	Error of Balance (g)	Uncertainty ± (mg)	Coverage factor *k*
Unload	0.0000	0.0000	0.0000	0.07	2,00
5.0000	5.0000	5.0000	0.0000	0.11	2,00
10.0000	10.0000	10.0001	+0.0001	0.11	2,00
20.0000	20.0000	20.0001	+0.0001	0.11	2,00
40.0000	40.0000	40.0001	+0.0001	0.13	2,00
60.0000	60.0000	60.0001	+0.0001	0.17	2,00
80.0000	80.0000	80.0002	+0.0002	0.17	2,00
100.0000	100.0000	100.0001	+0.0001	0.17	2,00
120.0000	120.0000	120.0001	+0.0001	0.29	2,00
140.0000	140.0000	140.0002	+0.0002	0.29	2,00
160.0000	160.0000	160.0002	+0.0002	0.29	2,00
180.0000	180.0000	180.0001	+0.0001	0.29	2,00
200.0000	200.0001	200.0001	0.0000	0.29	2,00

2. Repeatability of indications

Nominal Test Value (g)	Standard Deviation of Reading (g)
200.0000	0.00005

3. Effect of eccentric application of a load on the indication

☐ 

☑ 

Nominal Test Value (g)	Display Value (g)					Maximum Difference of Center Value (g)
	Position 1	Position 2	Position 3	Position 4	Position 5	
100.0000	100.0001	100.0001	100.0002	100.0002	100.0002	0.0001

Note. The Scope of Accredited TISI Certificate No. 23-LB0092 Issue 02 Page 116 of 138

This report is valid for the above stated instrument/s only.

End of Certificate

CALIBRATION LABORATORY CO., LTD.
2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com
CLC Accredited ISO/IEC 17025
NSC-TISI-TIS 17025 CALIBRATION 0059 CLC

REPORT OF CALIBRATION

FOR

NOMENCLATURE	:	**BALANCE**
MANUFACTURER	:	**SHIMADZU**
MODEL / TYPE	:	**AP225WD**
SERIAL NO.	:	**D316300692[LA-001]**
LOCATION SITE	:	**LABORATORY-BALANCE ROOM**
DATE OF CALIBRATION	:	**04 April 2024**

ENVIRONMENT CONDITIONS :

Temperature : 23 °C to 24 °C **Relative Humidity : 49 % to 50 %**

PROCEDURE USED :

This instrument was calibrated under procedure No. **WI-305-46** based on **EURAMET/cg-18/Version 4.0 (11/2015).**

The calibration was performed by Comparison with Weight Set which maintained by the Calibration Laboratory Co., Ltd.

REFERENCE STANDARD USED :

1. Weight Set, Phoenix Class E2 S/N. WBS-SET-E2-01.
2. Weight, Sartorius Class E2 S/N. 44329129, 43529037, 44329167, 43529293.

TRACEABILITY :

1. The measurements are traceable to International System of Units (SI), through National Institute of Metrology (Thailand). Certificate No. MM-0123-22, Due Date 22 August 2024.
2. The measurements are traceable to International System of Units (SI) , through Sartorius Lab Instruments GmbH & Co. KG. Certificate No. M141607, M141608, M141609, M141611. Due Date 15 September 2025.

UNCERTAINTY :

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor complies with the table which for a normal distribution corresponds to a coverage probability of approximately 95%. It has been evaluated according to the "Evaluation of the Uncertainty of Measurement in Calibration (EA-4/02 M:2022)"

CALIBRATION LABORATORY CO., LTD.
2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com

CLC Accredited ISO/IEC 17025

ilac-MRA

ANAB ANSI National Accreditation Board ACCREDITED ISO/IEC 17025 CALIBRATION AND DIMENSIONAL MEASUREMENT ACDM-2814

MM-C20

REPORT OF CALIBRATION

FOR

NOMENCLATURE	:	PRIMARY FLOW CALIBRATOR
MANUFACTURER	:	MESALABS
MODEL / TYPE	:	DEFENDER 510-M
SERIAL NO.	:	172525
DATE OF CALIBRATION	:	11 October 2024

ENVIRONMENT CONDITIONS :

Temperature : (23 ± 2) °C Relative Humidity : (55 ± 10) % RH

PROCEDURE USED :

This instrument was calibrated under procedure No. **CLC-CPPF-03.** The calibration was performed by comparison with Gas Flow Meter which refers to the standard condition of 101.325 kPa and 0 °C.

REFERENCE STANDARD USED :

Gas Flow Meter, Alicat Scientific Model M-5SLPM-D-DB15 S/N. 261330.

TRACEABILITY :

The measurements are traceable to International System of Units (SI), through Chell Intrument Ltd.

Certificate No. N037064, Due Date 26 February 2025.

UNCERTAINTY :

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor complies with the table which for a normal distribution corresponds to a coverage probability of approximately 95 %.

It has been evaluated according to the "Evaluation of the Uncertainty of Measurement in Calibration (EA-4/02 M:2022)"

@clccalibration

ม.17/21

CALIBRATION LABORATORY CO., LTD.
2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com

CLC Accredited ISO/IEC 17025

ilac-MRA

ANAB ANSI National Accreditation Board ACCREDITED ISO/IEC 17025 CALIBRATION AND DIMENSIONAL MEASUREMENT ACDM-2814

CERTIFICATE OF CALIBRATION

FOR

NOMENCLATURE	:	PRIMARY FLOW CALIBRATOR
MANUFACTURER	:	MESALABS
MODEL / TYPE	:	DEFENDER 510-M
SERIAL NO.	:	172525
CLID. NO.	:	212401789
JOB CONTROL NO.	:	241010108770
CALIBRATION SERVICE	:	☑ IN-LABORATORY ☐ ON-SITE

CUSTOMER : ENVIRONMENTAL MEASUREMENTS CO., LTD.
5/45 BAAN KLANG KRUNG BIZ TOWN, SOI SRINAGARINDRA 46/1 (PRAMOTE),
NONG BON SUB-DISTRICT, PRAWET DISTRICT, BANGKOK 10250

DATE OF RECEIVED : 10 October 2024 DATE OF ISSUED : 15 October 2024

The report of calibration shall not be reproduced except in full without approval of the Calibration Laboratory Co., Ltd.

Calibrated By :

Approved By :

15 October 2024

This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to the International System of Units (SI)

@clccalibration

MM-C20

JIRANATEE ASSOCIATES CO.,LTD.

Jiranatee Associates Co.,Ltd
63/14-15, 67/35-36
Petchkasem 7,7/1, Rd. Watthapra, Bangkokyai,
Bangkok 10600(Thailand)
Tel: +6608680812
Mobile: +66863999453
E-mail: jnac-calibration@jiranatee.com
Web site: www.jiranatee.com

Accredited calibration laboratory
ISO/IEC 17025:2017
NSC-TISI-TIS 17025
CALIBRATION 0367

Flow measurement laboratory
Calibration services department.

NSC – TISI – TIS 17025
CALIBRATION 0367

CERTIFICATE OF CALIBRATION

Certificate No. : **COF-042-67**

MEASUREMENT ITEM	: Top Load Orifice
MANUFACTURER	: Thermo Scientific
MODEL/TYPE	: G25A
SERIAL NUMBER	: 3375
ID NUMBER	: -
CONDITION AS-RECEIVED	: Used item
CUSTOMER	: Environmental Measurements Co., Ltd. 5/45 Baan Klang Krung Biz Town, Soi Srinagarindra 46/1 (Pramote), Nong Bon Sub-District Prawet District, Bangkok 10250
RECEIVED DATE	: 27 Sep 2024
MEASUREMENT DATE	: 08 Oct 2024
ISSUE DATE	: 08 Oct 2024

Calibration procedure:
The Orifice gas flow device was calibrated against Standard Rotary Displacement Meter (Roots Meter) Model G65/IMC/W2-dp. The WI-CL-004 was used as a calibration guideline.

Traceability:
This certificate provides a traceability of the measurement to recognized the national standards, and to realization of the international system of units (SI) through the NIMT (National Metrology Institute of Thailand) via Certificate number: MW-0063-23.

Uncertainty of Measurement:
The reported uncertainty of measurement is based on the standard uncertainty multiplied by a coverage factor k=2, Which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty has been determined in accordance with the GUM 'Evaluation of measurement data - Guide to the expression of uncertainty in measurement'

ENVIRONMENTAL CONDITIONS:
Ambient condition in the laboratory are as follow:

Temperature	: 23.0 ± 3.0	°C
Relative Humidity	: 55.0 ± 15.0	%RH
Atmospheric Pressure	: 1010 ± 10	hPa

CALIBRATION CONDITION:

Preconditioning	: 24 hours at ambient conditions.
Measurement Condition	: The average values during measurement are 23.7 °C and 52.7 %RH.

NOTED: *The certificate is valid only to the item calibrated on date and place of calibration.*

TABULATION OF RESULTS:
The table on next page give the measured values.

Calibrated by:

☐ Mr. Sorawit Thachalad
☑ Miss Jittraporn Lertsomphol

9.1.17/22

THIS CERTIFICATE REPORT MAY NOT BE REPRODUCED EXCEPT IN FULL UNLESS PERMISSION FOR REPRODUCTION HAS BEEN OBTAINED IN WRITING FROM THE LABORATORY

Jiranatee Associates Co., Ltd.

CLC Accredited ISO/IEC 17025

CALIBRATION LABORATORY CO., LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com

ANAB ACCREDITED CALIBRATION AND DIMENSIONAL MEASUREMENT ACDM-2814

CONDITION OF CALIBRATION ITEM : RECEIVED IN GOOD OPERATIONAL CONDITION

MEASUREMENT RESULTS : (X) without adjustment ( ) adjustment

The table in the following gives the calibration results and associated measurement uncertainties of the measuring primary flow calibrator.

CALIBRATION DATA

DUC Setting (L / min)	STD Reading (L / min)	Correction (L / min)	Uncertainty ± (L/min)
0.500	0.51828	+0.01828	0.57735
1.000	1.0326	+0.0326	0.5774
2.000	2.0561	+0.0561	0.5774
5.000	5.1183	+0.1183	0.5781

Technical Note. Media of Gas : Air

Setting Temperature 23 ° C ; Pressure 101.3 kPa

Note. The Scope of Accredited ANAB Certificate No. ACDM-2814 Version 012 Page 48 of 67

This report is valid for the above stated instrument/s only.

End of Certificate

Certificate No. Q24108770

F3-011-05/12-23

@clccalibration

MM-C20

THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804,0-2399-0469

Calibration Certificate

Issued by : Calibration & Test Section : Meteorological Instruments Bureau

Date of Issue 3 October, 2023 Certification No. 344/23

Page : 1 of 2

Object : Wind speed and wind direction

Manufacturer : Sensor : NRG

Basic Datalogger : Symphonie

Type : Sensor : 40C Basic Datalogger : LR20

Serial No. : Sensor : 1795-00135858 Basic Datalogger : 309013229

Customer : Environmental Measurements Co.,Ltd.
5/45 Baan Klang Krung Biz Town, Soi Srinagarindra 46/1 (Pramote),
Nong Bon Sub-District, Prawet District, Bangkok 10250.

Calibration Condition : Temperature 25.1 °C Barometric Pressure 1011.3 hPa

NATIONAL STANDARD WIND TUNNEL :

: Thermal Anemometer 642 S/N 91563

: HOOK GAGE NO 1425 Pitot Tube Theodor Friedrichs Type 0800.0000 serial 9023

N.I.S.T. Test Reference Number 731/241460 : Standard Velocity at 20 - 30 m/sec

: Ultrasonic Anemometer Model DA-650-3TV (sensor TR-90AH)

Serial Number 110730029 (sensor 120629586)

JAPAN QUALITY ASSURANCE ORGANIZATION : Standard Velocity at 0 - 20 m/sec

ised Signatory)
the Chief
dard Instrument

OLOGICAL DEPARTMENT

พ.17/23

JIRANATEE ASSOCIATES CO.,LTD.

MEASUREMENT RESULTS:

The Orifice gas flow device was calibrated by direct comparison method with the Standard Rotary Displacement Meter (Roots Meter). The Humid air was used as a medium in the system. The standard conditions are 25°C (298.15 K) and 760 mmHg for standard temperature and standard pressure respectively.

Table 1: The results of Q Standard calibration data

Plate	Flow rate m³/min	Pressure [Pa] mmHg	Temperature [Ta] °C	Temperature [Tm] °C	Δp_meter mmHg	Δp_Orifice inH₂O	Y	Standard Flow [Q_s] m³/min
1	0.702	757.395	23.63	22.54	57.122	1.729	1.316	0.653
2	1.000	757.471	23.83	22.84	61.580	3.472	1.864	0.923
3	1.119	757.263	23.92	22.82	43.090	4.596	2.144	1.059
4	1.165	757.228	23.85	22.65	30.341	5.160	2.272	1.123
5	1.409	757.252	23.68	22.47	30.293	7.615	2.761	1.359

Slope (m): **2.04447**

Intercept (b): **-0.02098**

Correlation coefficient (r): **0.99989**

Uncertainty (k=2): **0.015** m³/min

Table 2: The results of Q actual calibration data

Plate	Flow rate m³/min	Pressure [Pa] mmHg	Temperature [Ta] °C	Temperature [Tm] °C	Δp_meter mmHg	Δp_Orifice inH₂O	Y	Standard Flow [Q_a] m³/min
1	0.702	757.395	23.63	22.54	57.122	1.729	0.823	0.652
2	1.000	757.471	23.83	22.84	61.580	3.472	1.167	0.922
3	1.119	757.263	23.92	22.82	43.090	4.596	1.343	1.059
4	1.165	757.228	23.85	22.65	30.341	5.160	1.423	1.123
5	1.409	757.252	23.68	22.47	30.293	7.615	1.728	1.358

Slope (m): **1.28051**

Intercept (b): **-0.01311**

Correlation coefficient (r): **0.99989**

Uncertainty (k = 2): **0.015** m³/min

End of Certificate of Calibration

Jiranatee Associates Co., Ltd.

MM-C20

CALIBRATION LABORATORY CO., LTD.
2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com

CLC Accredited ISO/IEC 17025

NSC-TISI-TIS 17025
CALIBRATION 0059
CLC

CERTIFICATE OF CALIBRATION

FOR

NOMENCLATURE	:	VIBRATION METER
MANUFACTURER	:	VIBROCK
MODEL / TYPE	:	V9000
SERIAL NO.	:	2351
CLID. NO.	:	252101273
JOB CONTROL NO.	:	240912097767
CALIBRATION SERVICE	:	☑ IN-LABORATORY ☐ ON-SITE

CUSTOMER : ENVIRONMENTAL MEASUREMENTS CO., LTD.
5/45 BAAN KLANG KRUNG BIZ TOWN, SOI SRINAGARINDRA 46/1 (PRAMOTE),
NONG BON SUB-DISTRICT, PRAWET DISTRICT, BANGKOK 10250

DATE OF RECEIVED : 12 September 2024 DATE OF ISSUED : 16 September 2024

The report of calibration shall not be reproduced except in full without approval of the Calibration Laboratory Co., Ltd.

Calibrated By :

Approved By :

16 September 2024

This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to the International System of Units (SI)

Certificate No. Q24097767
F3-011-05/12-23

@clccalibration

พ.17/24

THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804,0-2399-0469

The Result of Calibration

Certification No. 344/23

3 October, 2023

Standard	HOOK GAGE NO. 1425			TESTED ANEMOMETER	
Ultrasonic Anemometer	Pressure	Vacumm	Velocity	Velocity	Correction
m/sec	inches H2O	inches H2O	m/sec	m/sec	m/sec
1.00	-	-	-	0.95	0.05
3.02	-	-	-	2.85	0.17
5.00	-	-	-	4.95	0.05
7.00	-	-	-	6.85	0.15
9.02	-	-	-	8.95	0.07
11.01	-	-	-	10.85	0.16
13.01	-	-	-	12.99	0.02
15.01	-	-	-	15.10	-0.09
17.02	-	-	-	16.98	0.04
20.02	-	-	-	20.13	-0.11

Wind Aloft Plotting Board. US.DEPARTMENT OF COMMERCE WEATHER BUREAU	
WIND DIRETION	TESTED WIND DIRECTION
0	0
90	90
180	180
270	270

CALIBRATION LABORATORY CO., LTD.
2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com
CLC Accredited ISO/IEC 17025
NSC-TISI-TIS 17025 CALIBRATION 0059 CLC

CONDITION OF CALIBRATION ITEM : RECEIVED IN GOOD OPERATIONAL CONDITION

MEASUREMENT RESULTS : (X) without adjustment ( ) adjustment

CALIBRATION DATA

VELOCITY RESULT

Test point		Mode	STD Reading	DUC Reading	Correction	Uncertainty
(mm/s)	(frequency)		(mm/s)	(mm/s)	(mm/s)	± (% of rdg.)
10	160 Hz	peak	10.00	9.82	+0.18	1.1
20	160 Hz		20.00	19.44	+0.56	1.0
40	160 Hz		40.00	39.23	+0.77	1.0
60	160 Hz		60.00	58.94	+1.06	1.0
80	160 Hz		80.00	78.55	+1.45	1.0
100	160 Hz		100.00	97.49	+2.51	1.0

Note. The Scope of Accredited TISI Certificate No. 23-LB0092 Issue 02 Page 60 of 138

This report is valid for the above stated instrument/s only.

End of Certificate

CALIBRATION LABORATORY CO., LTD.
2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com
CLC Accredited ISO/IEC 17025
NSC-TISI-TIS 17025 CALIBRATION 0059 CLC

REPORT OF CALIBRATION

FOR

NOMENCLATURE	:	**VIBRATION METER**
MANUFACTURER	:	**VIBROCK**
MODEL / TYPE	:	**V9000**
SERIAL NO.	:	**2351**
DATE OF CALIBRATION	:	**13 September 2024**

ENVIRONMENT CONDITIONS :

Temperature : (23 ± 2) °C **Relative Humidity :** (55 ± 15) %RH

PROCEDURE USED :

This instrument was calibrated under procedure No. **WI-305-127** based on **ISO 16063-21** as calibration guideline.

The calibration was performed by using Digital Multimeter, Programmable Timer/Counter, Accelerometer and Measuring Amplifier which maintained by the Calibration Laboratory Co., Ltd.

REFERENCE STANDARD USED :

1. Digital Multimeter, Hewlett Packard Model 34401A S/N. 3146A75935.
2. Programmable Timer/Counter, Philips Model PM6680B S/N. SM607101.
3. Accelerometer with Measuring Amplifier, Bruel & Kjaer Model 8305, 2626 S/N. 705491, 1741406.

TRACEABILITY :

1. The measurements are traceable to International System of Units (SI), through National Institute of Metrology (Thailand) Certificate No. EE-0130-23, Due Date 29 November 2024.
2. The measurements are traceable to International System of Units (SI), through Aeronautical Radio of Thailand Ltd. Certificate No. 07-0050/24 , Due Date 13 May 2025 .
3. The measurements are traceable to International System of Units (SI), through National Institute of Metrology (Thailand) Certificate No. AV-0053-23, Due Date 12 October 2024.

UNCERTAINTY :

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k = 2,00 which for a normal distribution corresponds to a coverage probability of approximately 95 %. It has been evaluated according to the "Evaluation of the Uncertainty of Measurement in Calibration (EA-4/02 M:2022)"

MM-C20

Certificate No.: C2409-0836

	Pressure:	Temperature:	Relative humidity:
Environmental conditions:			
Reference conditions:	101.325 kPa	23.0 °C	50 %RH
Measurement conditions:	100.90 ± 0.01 kPa	23.2 ± 1.1 °C	58.2 ± 2.3 %RH

1. Sound pressure level

Specified sound pressure level (dB)	Measured sound pressure level (dB)	Deviated value (dB)	Tolerance limit IEC60942:2017 Class 1 (dB)
Reference microphone 40AU S/N 309231			
94.00	93.93	0.07	±0.25
114.00	114.01	0.01	±0.25

2. Frequency

Specified Frequency (Hz)	Measured Frequency (Hz)	Deviated value (%)	Tolerance limit IEC60942:2017 Class 1 (%)
Reference microphone 40AU S/N 309231			
1000.00	1000.30	0.03	±0.7
1000.00	1000.18	0.02	±0.7

3. Total distortion + Noise

Specified sound pressure level (dB)	Measured Distortion (%)	Tolerance limit IEC60942:2017 Class 1 (%)
Reference Sound Analyser Nor140 S/N 1405248		
94.00	0.50	±2.5
114.00	1.10	±2.5

Uncertainty of measurement

Parameters	Uncertainty
Sound pressure level	0.10 dB
Frequency	0.020 %
Total distortion + Noise	0.10 %

Date of calibration: 2024-09-30
Date of issue : 2024-10-02

9.17/26

Acoustic Laboratory (Thailand) Co., Ltd.
6/57 Soi Phoem Sin 42, Sai Mai, Sai Mai, Bangkok 10220
Tel: (+66) 02-1296780 Email: info@altbkk.com

NSC-TISI-TIS 17025 CALIBRATION 0468

Certificate of Calibration

Certificate No.: C2409-0836

Customer: ENVIRONMENTAL MEASUREMENTS CO., LTD.
5/45 Baan Klang Krung Biz Town, Soi Srinagarindra
46/1 (Pramote), NONG BON Sub-district,
PRAWET District, BANGKOK 10250

Date of calibration: 2024-09-30
Date of issue: 2024-10-02
Instrument Calibrated: Sound Calibrator
Manufacturer: BSWA
Type: CA111
Serial no: 550482

Calibration and verification performed:
The performed tests refer to IEC 60942 (2017): Electro-acoustics - Sound Calibrators. The calibrator has been tested as described in Annex B of the same standard.

Preconditioning:
The equipment was preconditioned for more than 16 hours at the specified calibration temperature and humidity

Instruments and Program:
A complete list of instruments, hardware, and software, that has been used for this calibration is separately available from the calibration laboratory.

Equipment standards used:
-Sound Measuring Equipment Calibration Unit 483B S/N31083
-Digital Multimeter Keysight S/N HP34401A
-Ultra-low Distortion Function Generator Stanford SRS DS360 S/N123625
-Acoustic Sound Calibrator Class 0 Nor1253 S/N32941
-Reference Microphone Condenser G.R.A.S. 40AU-1 S/N309231
-Sound Analyser Nor140 S/N1405248
-Combined Pressure, Humidity and Temperature Transmitter PTU300 S/NM2520568

Traceability
The measured values are traceable to following the ISO/IEC 17025 laboratories:
Sound Pressure Level: NCL, Norway
Reference microphone: NCL, Norway
Voltage: TPA, Thailand
Frequency: TPA, Thailand
Reference Pressure, Humidity and Temperature: TPA, Thailand
Distortion Meter: EEI,Thailand

This certificate of calibration is issued by Acoustic Laboratory Thailand (ALT). It also states that the laboratory has a satisfactory quality assurance system and traceability to accredited or national calibration laboratories. This certificate may not be reproduced other than in full.

MM-C20

Request No. : 22-68 / 0059

MTC No. : PSL-P 0019 / 68

CERTIFICATE OF CALIBRATION

Nomenclature : Digital Lux Meter

Serial No. : A.067438

Maker : EXTECH Instruments

Model : 407026

Customer : **ENVIRONMENTAL MEASUREMENTS CO., LTD.**

Address : 5/45 Baan Klang Krung Biz Town, Soi Srinagarindra 46/1 (Pramote), Nong Bon Sub-District Prawet District, Bangkok 10250

Date of receipt : 28 October 2024

Date of calibration : 4 November 2024

Place of calibration : Photometry and Temperature Standards Laboratory, MTC. (Bangpoo)

Basis of calibration : calibration at 0 ~ 5000 lux.

Condition of calibration : - Ambient temperature : (25 ± 2) °C

- Relative humidity : (60 ± 20) %

Reference Standard : Working Standard Luminous Intensity Lamp, Serial No.: FEL003 and 3501, can be traceable to international system of units (SI), through calibration certificate MTC No. PSL-P 0151/67 and PSL-P 0152/67, date of calibration 10 May 2024.

Traceability : This certificate is traceable to SI units through the National Institute of Metrology (Thailand) calibration certificate No. TP-1010-23, TP-1011-23 and TP-1012-23

Support Equipment : 1. Photometric bench , 3.0 meter long

2. DC power supply, Serial No.: BC - 341006035007/2

3. Digital Multimeter , Model : R 6551 , S/N : 92041186 and 92041192

Calibration Procedure : The measurement was done in accordance with WI.CP.10.

The reported uncertainty is based on a standard uncertainty multiplied by a coverage factor k = 2 , providing a level of confidence of approximately 95 %.

R.P.

The results relate only to the items tested/calibrated or value assigned.
Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

Acoustic Laboratory Thailand

Certificate No.: C2409-0836

The reported expanded uncertainty is based upon a standard uncertainty multiplied by a coverage factor k = 2, providing a level of confidence of approximately 95%

Date of calibration: 2024-09-30

Date of issue : 2024-10-02

-------- End of Calibration Certificate -------

ALT
Acoustic Laboratory Thailand

MM-C20

Acoustic Laboratory (Thailand) Co., Ltd.
6/57 Soi Phoem Sin 42, Sai Mai, Sai Mai, Bangkok 10220
Tel: (+66) 02-1296780 Email: info@altbkk.com

Certificate of Calibration

Certificate No.: S2409-0833

Customer: ENVIRONMENTAL MEASUREMENTS CO., LTD.
5/45 Baan Klang Krung Biz Town, Soi Srinagarindra
46/1 (Pramote), NONG BON Sub-district,
PRAWET District, BANGKOK 10250

Date of calibration: 2024-10-01
Date of issue: 2024-10-02
Instrument Calibrated: Noise Dosimeter
Manufacturer: SOUNDTEK
Model: ST-130
Serial no: 170800130

Calibration and verification performed:
Acoustical levels are stated relative to 20µPa. Other dB levels are relative values.
The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k, which with the reported effective degree of freedom corresponds to coverage probability of approximately 95%.
The sound level meter instrument submitted for periodic testing following the periodic tests of IEC 61672-3 : 2013.

Preconditioning:
The equipment was preconditioned for more than 16 hours at the specified calibration temperature and humidity.

Instruments and Program:
A complete list of instruments, hardware, and software, that has been used for this calibration is separately available from the calibration laboratory.

Equipment standards used:
- Sound measuring equipment calibration unit Nor140 S/N1405248
- Acoustic sound calibrator class 1 Nor1256 S/N125626542
- Combined Pressure, Humidity and Temperature Transmitter PTU300 S/NM2520568

Traceability
The measured values are traceable to following the ISO/IEC 17025 laboratories:
Sound Pressure Level: EEI, Thailand
Reference Pressure, Humidity and Temperature: TPA, Thailand

This certificate of calibration is issued by Acoustic Laboratory Thailand (ALT). It also states that the laboratory has a satisfactory quality assurance system and traceability to accredited or national calibration laboratories. This certificate may not be reproduced other than in full.

Request No. : 22-68 / 0059
MTC No. : PSL-P 0019 / 68
Serial No. : A.067438

Results :

UUC Range (lux)	Standard (lux)	*UUC Reading Before Adj.(lux)	UUC Reading After Adj.(lux)	Uncertainty of Measurement ± (lux)
2000	100	103	104	2.0
	500	502	505	10
	1000	992	1000	20
	1500	1486	1497	30
	2000	1972	1994	40
20000 (×10)	2000	197	200	40
	3000	296	300	60
	4000	391	397	80
	5000	490	497	100

Note : *UUC = Unit Under Calibration.

...end of certificate...

The results relate only to the items tested/calibrated or value assigned.
Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

Certificate No.: S2409-0833

C-Weighting acoustic frequency response meter free-field acoustic response at a level of 80.0 dB

Frequency Weighting (Hz)	Deviation from various frequency weighting response curve		
	C-Weighting (dB)	Uncertainty (dB)	Acceptance limit (dB)
125	0.4	0.20	±1.5
1000	0.0	0.20	±1.0
8000	1.3	0.20	±5.0

Note: Acoustical signal test of frequency weightings are not accredited

The reported expanded uncertainty is based upon a standard uncertainty multiplied by a coverage factor k = 2, providing a level of confidence of approximately 95%

Date of calibration : 2024-10-01
Date of issue : 2024-10-02

-------- End of Calibration Certificate -------

ALT Acoustic Laboratory Thailand

Certificate No.: S2409-0833

Environmental conditions:	Pressure:	Temperature:	Relative humidity:
Reference conditions:	101.325 kPa	23.0 °C	50 %RH
Measurement conditions:	100.78 ± 0.10 kPa	22.9 ± 0.5 °C	52.5 ± 5.0 %RH

1. Indication at the calibration check frequency

Reference Acoustic Signal (dB)	Measured value (dB)		Deviated value (dB)	Uncertainty (dB)	Acceptant limit (dB)
	Before adjust	After adjust			
93.9	94.1	93.9	0.0	0.12	±1.0

Note: Indication at the checked calibration frequency was adjusted to 93.9 dB by the sound calibrator BSWA model:CA111 S/N:550482

2. Frequency Weighting at 1 kHz

Frequency Weighting	Measured value (dB)	Deviated value (dB)	Uncertainty (dB)	Acceptance limit (dB)
A-Weighting	94.0	0.0	0.20	±0.3
C-Weighting	94.0	0.0	0.20	±0.3

Note: Frequency weighting at 1 kHz are not accredited

3. Time Weighting at 1 kHz

Time Weighting	Measured value (dB)	Deviated value (dB)	Uncertainty (dB)	Acceptance limit (dB)
Fast	94.0	0.0	0.20	±0.3
Slow	94.0	0.0	0.20	±0.3

Note: Time Weighting at 1 kHz are not accredited

4. Acoustical signal test of frequency weightings

A-Weighting acoustic frequency response meter free-field acoustic response at a level of 80.0 dB

Frequency Weighting (Hz)	Deviation from various frequency weighting response curve		
	A-Weighting (dB)	Uncertainty (dB)	Acceptance limit (dB)
125	0.2	0.20	±1.5
1000	0.0	0.20	±1.0
8000	0.6	0.20	±5.0

Note: Acoustical signal test of frequency weightings are not accredited

Date of calibration : 2024-10-01
Date of issue : 2024-10-02

Acoustic Laboratory (Thailand) Co., Ltd.
6/57 Soi Phoem Sin 42, Sai Mai, Sai Mai, Bangkok 10220
Tel: (+66) 02-1296780 Email: info@altbkk.com

Certificate of Calibration

Certificate No.: S2409-0834

Customer: ENVIRONMENTAL MEASUREMENTS CO., LTD.
5/45 Baan Klang Krung Biz Town, Soi Srinagarindra
46/1 (Pramote), NONG BON Sub-district,
PRAWET District, BANGKOK 10250

Date of calibration: 2024-10-01
Date of issue: 2024-10-02
Instrument Calibrated: Noise Dosimeter
Manufacturer: SOUNDTEK
Model: ST-130
Serial no: 170800167

Calibration and verification performed:
Acoustical levels are stated relative to 20µPa. Other dB levels are relative values.
The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k, which with the reported effective degree of freedom corresponds to coverage probability of approximately 95%.
The sound level meter instrument submitted for periodic testing following the periodic tests of IEC 61672-3 : 2013.

Preconditioning:
The equipment was preconditioned for more than 16 hours at the specified calibration temperature and humidity.

Instruments and Program:
A complete list of instruments, hardware, and software, that has been used for this calibration is separately available from the calibration laboratory.

Equipment standards used:
- Sound measuring equipment calibration unit Nor140 S/N1405248
- Acoustic sound calibrator class 1 Nor1256 S/N125626542
- Combined Pressure, Humidity and Temperature Transmitter PTU300 S/NM2520568

Traceability
The measured values are traceable to following the ISO/IEC 17025 laboratories:
Sound Pressure Level: EEI, Thailand
Reference Pressure, Humidity and Temperature: TPA, Thailand

This certificate of calibration is issued by Acoustic Laboratory Thailand (ALT). It also states that the laboratory has a satisfactory quality assurance system and traceability to accredited or national calibration laboratories. This certificate may not be reproduced other than in full.

Certificate No.: S2409-0834

Environmental conditions:	Pressure:	Temperature:	Relative humidity:
Reference conditions:	101.325 kPa	23.0 °C	50 %RH
Measurement conditions:	100.38 ± 0.50 kPa	23.0 ± 0.5 °C	53.4 ± 5.0 %RH

1. Indication at the calibration check frequency

Reference Acoustic Signal (dB)	Measured value (dB)		Deviated value (dB)	Uncertainty (dB)	Acceptant limit (dB)
	Before adjust	After adjust			
93.9	94.1	93.9	0.0	0.12	±1.0

Note: Indication at the checked calibration frequency was adjusted to 93.9 dB by the sound calibrator BSWA model:CA111 S/N:550482

2. Frequency Weighting at 1 kHz

Frequency Weighting	Measured value (dB)	Deviated value (dB)	Uncertainty (dB)	Acceptance limit (dB)
A-Weighting	94.0	0.0	0.20	±0.3
C-Weighting	93.9	0.0	0.20	±0.3

Note: Frequency weighting at 1 kHz are not accredited

3. Time Weighting at 1 kHz

Time Weighting	Measured value (dB)	Deviated value (dB)	Uncertainty (dB)	Acceptance limit (dB)
Fast	94.0	0.0	0.20	±0.3
Slow	94.0	0.0	0.20	±0.3

Note: Time Weighting at 1 kHz are not accredited

4. Acoustical signal test of frequency weightings

A-Weighting acoustic frequency response meter free-field acoustic response at a level of 80.0 dB

Frequency Weighting (Hz)	Deviation from various frequency weighting response curve		
	A-Weighting (dB)	Uncertainty (dB)	Acceptance limit (dB)
125	0.1	0.20	±1.5
1000	0.0	0.20	±1.0
8000	1.9	0.20	±5.0

Note: Acoustical signal test of frequency weightings are not accredited

Date of calibration : 2024-10-01
Date of Issue : 2024-10-02

MM-C20

Acoustic Laboratory (Thailand) Co., Ltd.
6/57 Soi Phoem Sin 42, Sai Mai, Sai Mai, Bangkok 10220
Tel: (+66) 02-1296780 Email: info@altbkk.com

Certificate of Calibration

Certificate No.: S2409-0835

Customer: ENVIRONMENTAL MEASUREMENTS CO., LTD.
5/45 Baan Klang Krung Biz Town, Soi Srinagarindra
46/1 (Pramote), NONG BON Sub-district,
PRAWET District, BANGKOK 10250

Date of calibration: 2024-10-01
Date of issue: 2024-10-02
Instrument Calibrated: Noise Dosimeter
Manufacturer: SOUNDTEK
Model: ST-130
Serial no: 170800266

Calibration and verification performed:
Acoustical levels are stated relative to 20µPa. Other dB levels are relative values.
The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k, which with the reported effective degree of freedom corresponds to coverage probability of approximately 95%.
The sound level meter instrument submitted for periodic testing following the periodic tests of IEC 61672-3 : 2013.

Preconditioning:
The equipment was preconditioned for more than 16 hours at the specified calibration temperature and humidity.

Instruments and Program:
A complete list of instruments, hardware, and software, that has been used for this calibration is separately available from the calibration laboratory.

Equipment standards used:
- Sound measuring equipment calibration unit Nor140 S/N1405248
- Acoustic sound calibrator class 1 Nor1256 S/N125626542
- Combined Pressure, Humidity and Temperature Transmitter PTU300 S/NM2520568

Traceability
The measured values are traceable to following the ISO/IEC 17025 laboratories:
Sound Pressure Level: EEI, Thailand
Reference Pressure, Humidity and Temperature: TPA, Thailand

This certificate of calibration is issued by Acoustic Laboratory Thailand (ALT). It also states that the laboratory has a satisfactory quality assurance system and traceability to accredited or national calibration laboratories. This certificate may not be reproduced other than in full.

ม.17/31

C-Weighting acoustic frequency response meter free-field acoustic response at a level of 80.0 dB

Frequency Weighting (Hz)	Deviation from various frequency weighting response curve		
	C-Weighting (dB)	Uncertainty (dB)	Acceptance limit (dB)
125	1.0	0.20	±1.5
1000	-0.1	0.20	±1.0
8000	2.5	0.20	±5.0

Note: Acoustical signal test of frequency weightings are not accredited

The reported expanded uncertainty is based upon a standard uncertainty multiplied by a coverage factor k = 2, providing a level of confidence of approximately 95%

Date of calibration : 2024-10-01
Date of issue : 2024-10-02

------- End of Calibration Certificate -------

ALT Acoustic Laboratory Thailand

Certificate No.: S2409-0835

C-Weighting acoustic frequency response meter free-field acoustic response at a level of 80.0 dB

Frequency Weighting (Hz)	Deviation from various frequency weighting response curve		
	C-Weighting (dB)	Uncertainty (dB)	Acceptance limit (dB)
125	0.5	0.20	±1.5
1000	0.3	0.20	±1.0
8000	4.5	0.20	±5.0

Note: Acoustical signal test of frequency weightings are not accredited

The reported expanded uncertainty is based upon a standard uncertainty multiplied by a coverage factor k = 2, providing a level of confidence of approximately 95%

Date of calibration : 2024-10-01
Date of issue : 2024-10-02

-------- End of Calibration Certificate -------

ALT Acoustic Laboratory Thailand

Certificate No.: S2409-0835

Environmental conditions:	Pressure:	Temperature:	Relative humidity:
Reference conditions:	101.325 kPa	23.0 °C	50 %RH
Measurement conditions:	100.38 ± 0.50 kPa	23.0 ± 0.5 °C	53.4 ± 5.0 %RH

1. Indication at the calibration check frequency

Reference Acoustic Signal (dB)	Measured value (dB)		Deviated value (dB)	Uncertainty (dB)	Acceptant limit (dB)
	Before adjust	After adjust			
93.9	94.1	93.9	0.0	0.12	±1.0

Note: Indication at the checked calibration frequency was adjusted to 93.9 dB by the sound calibrator BSWA model:CA111 S/N:550482

2. Frequency Weighting at 1 kHz

Frequency Weighting	Measured value (dB)	Deviated value (dB)	Uncertainty (dB)	Acceptance limit (dB)
A-Weighting	94.0	0.0	0.20	±0.3
C-Weighting	94.1	0.0	0.20	±0.3

Note: Frequency weighting at 1 kHz are not accredited

3. Time Weighting at 1 kHz

Time Weighting	Measured value (dB)	Deviated value (dB)	Uncertainty (dB)	Acceptance limit (dB)
Fast	94.0	0.0	0.20	±0.3
Slow	94.0	0.0	0.20	±0.3

Note: Time Weighting at 1 kHz are not accredited

4. Acoustical signal test of frequency weightings

A-Weighting acoustic frequency response meter free-field acoustic response at a level of 80.0 dB

Frequency Weighting (Hz)	Deviation from various frequency weighting response curve		
	A-Weighting (dB)	Uncertainty (dB)	Acceptance limit (dB)
125	0.9	0.20	±1.5
1000	0.2	0.20	±1.0
8000	3.3	0.20	±5.0

Note: Acoustical signal test of frequency weightings are not accredited

Date of calibration : 2024-10-01
Date of issue : 2024-10-02

Acoustic Laboratory (Thailand) Co., Ltd.
6/57 Soi Phoem Sin 42, Sai Mai, Sai Mai, Bangkok 10220
Tel: (+66) 02-1296780 Email: info@altbkk.com

Certificate of Calibration

Certificate No.: S2409-0831

Customer: ENVIRONMENTAL MEASUREMENTS CO., LTD.
5/45 Baan Klang Krung Biz Town, Soi Srinagarindra
46/1 (Pramote), NONG BON Sub-district,
PRAWET District, BANGKOK 10250

Date of calibration: 2024-10-02
Date of issue: 2024-10-03
Instrument Calibrated: Noise Dosimeter
Manufacturer: SOUNDTEK
Model: ST-130
Serial no: 170800271

Calibration and verification performed:
Acoustical levels are stated relative to 20μPa. Other dB levels are relative values.
The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k, which with the reported effective degree of freedom corresponds to coverage probability of approximately 95%.
The sound level meter instrument submitted for periodic testing following the periodic tests of IEC 61672-3 : 2013.

Preconditioning:
The equipment was preconditioned for more than 16 hours at the specified calibration temperature and humidity.

Instruments and Program:
A complete list of instruments, hardware, and software, that has been used for this calibration is separately available from the calibration laboratory.

Equipment standards used:
- Sound measuring equipment calibration unit Nor140 S/N1405248
- Acoustic sound calibrator class 1 Nor1256 S/N125626542
- Combined Pressure, Humidity and Temperature Transmitter PTU300 S/NM2520568

Traceability
The measured values are traceable to following the ISO/IEC 17025 laboratories:
Sound Pressure Level: EEI, Thailand
Reference Pressure, Humidity and Temperature: TPA, Thailand

This certificate of calibration is issued by Acoustic Laboratory Thailand (ALT). It also states that the laboratory has a satisfactory quality assurance system and traceability to accredited or national calibration laboratories. This certificate may not be reproduced other than in full.

Certificate No.: S2409-0831

Environmental conditions:	Pressure:	Temperature:	Relative humidity:
Reference conditions:	101.325 kPa	23.0 °C	50 %RH
Measurement conditions:	100.38 ± 0.50 kPa	23.0 ± 0.5 °C	53.4 ± 5.0 %RH

1. Indication at the calibration check frequency

Reference Acoustic Signal (dB)	Measured value (dB)		Deviated value (dB)	Uncertainty (dB)	Acceptant limit (dB)
	Before adjust	After adjust			
93.9	93.8	93.9	0.0	0.12	±1.0

Note: Indication at the checked calibration frequency was adjusted to 93.9 dB by the sound calibrator BSWA model:CA111 S/N:550482

2. Frequency Weighting at 1 kHz

Frequency Weighting	Measured value (dB)	Deviated value (dB)	Uncertainty (dB)	Acceptance limit (dB)
A-Weighting	94.0	0.0	0.20	±0.3
C-Weighting	94.0	0.0	0.20	±0.3

Note: Frequency weighting at 1 kHz are not accredited

3. Time Weighting at 1 kHz

Time Weighting	Measured value (dB)	Deviated value (dB)	Uncertainty (dB)	Acceptance limit (dB)
Fast	94.0	0.0	0.20	±0.3
Slow	94.0	0.0	0.20	±0.3

Note: Time Weighting at 1 kHz are not accredited

4. Acoustical signal test of frequency weightings

A-Weighting acoustic frequency response meter free-field acoustic response at a level of 80.0 dB

Frequency Weighting (Hz)	Deviation from various frequency weighting response curve		
	A-Weighting (dB)	Uncertainty (dB)	Acceptance limit (dB)
125	-0.7	0.20	±1.5
1000	0.0	0.20	±1.0
8000	-0.4	0.20	±5.0

Note: Acoustical signal test of frequency weightings are not accredited

Date of calibration : 2024-10-02
Date of issue : 2024-10-03

MM-C20

Acoustic Laboratory (Thailand) Co., Ltd.
6/57 Soi Phoem Sin 42, Sai Mai, Sai Mai, Bangkok 10220
Tel: (+66) 02-1296780 Email: info@altbkk.com

Certificate of Calibration

Certificate No.: S2409-0832

Customer: ENVIRONMENTAL MEASUREMENTS CO., LTD.
5/45 Baan Klang Krung Biz Town, Soi Srinagarindra
46/1 (Pramote), NONG BON Sub-district,
PRAWET District, BANGKOK 10250

Date of calibration: 2024-10-01
Date of issue: 2024-10-02
Instrument Calibrated: Noise Dosimeter
Manufacturer: SOUNDTEK
Model: ST-130
Serial no: 170800288

Calibration and verification performed:
Acoustical levels are stated relative to 20μPa. Other dB levels are relative values.
The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k, which with the reported effective degree of freedom corresponds to coverage probability of approximately 95%.
The sound level meter instrument submitted for periodic testing following the periodic tests of IEC 61672-3 : 2013.

Preconditioning:
The equipment was preconditioned for more than 16 hours at the specified calibration temperature and humidity.

Instruments and Program:
A complete list of instruments, hardware, and software, that has been used for this calibration is separately available from the calibration laboratory.

Equipment standards used:
- Sound measuring equipment calibration unit Nor140 S/N1405248
- Acoustic sound calibrator class 1 Nor1256 S/N125626542
- Combined Pressure, Humidity and Temperature Transmitter PTU300 S/NM2520568

Traceability
The measured values are traceable to following the ISO/IEC 17025 laboratories:
Sound Pressure Level: EEI, Thailand
Reference Pressure, Humidity and Temperature: TPA, Thailand

This certificate of calibration is issued by Acoustic Laboratory Thailand (ALT). It also states that the laboratory has a satisfactory quality assurance system and traceability to accredited or national calibration laboratories. This certificate may not be reproduced other than in full.

Certificate No.: S2409-0831

C-Weighting acoustic frequency response meter free-field acoustic response at a level of 80.0 dB

Frequency Weighting (Hz)	Deviation from various frequency weighting response curve		
	C-Weighting (dB)	Uncertainty (dB)	Acceptance limit (dB)
125	-0.1	0.20	±1.5
1000	0.0	0.20	±1.0
8000	-0.3	0.20	±5.0

Note: Acoustical signal test of frequency weightings are not accredited

The reported expanded uncertainty is based upon a standard uncertainty multiplied by a coverage factor k = 2, providing a level of confidence of approximately 95%

(

Date of calibration : 2024-10-02
Date of issue : 2024-10-03

------- End of Calibration Certificate -------

ALT Acoustic Laboratory Thailand

Certificate No.: S2409-0832

C-Weighting acoustic frequency response meter free-field acoustic response at a level of 80.0 dB

Frequency Weighting (Hz)	Deviation from various frequency weighting response curve		
	C-Weighting (dB)	Uncertainty (dB)	Acceptance limit (dB)
125	0.1	0.20	±1.5
1000	0.1	0.20	±1.0
8000	3.0	0.20	±5.0

Note: Acoustical signal test of frequency weightings are not accredited

The reported expanded uncertainty is based upon a standard uncertainty multiplied by a coverage factor k = 2, providing a level of confidence of approximately 95%

(

Date of calibration : 2024-10-01
Date of issue : 2024-10-02

-------- End of Calibration Certificate -------

ALT Acoustic Laboratory Thailand

Certificate No.: S2409-0832

Environmental conditions:	Pressure:	Temperature:	Relative humidity:
Reference conditions:	101.325 kPa	23.0 °C	50 %RH
Measurement conditions:	100.38 ± 0.50 kPa	23.0 ± 0.5 °C	53.4 ± 5.0 %RH

1. Indication at the calibration check frequency

Reference Acoustic Signal (dB)	Measured value (dB)		Deviated value (dB)	Uncertainty (dB)	Acceptant limit (dB)
	Before adjust	After adjust			
93.9	93.6	93.9	0.0	0.12	±1.0

Note: Indication at the checked calibration frequency was adjusted to 93.9 dB by the sound calibrator BSWA model:CA111 S/N:550482

2. Frequency Weighting at 1 kHz

Frequency Weighting	Measured value (dB)	Deviated value (dB)	Uncertainty (dB)	Acceptance limit (dB)
A-Weighting	94.0	0.0	0.20	±0.3
C-Weighting	94.1	0.0	0.20	±0.3

Note: Frequency weighting at 1 kHz are not accredited

3. Time Weighting at 1 kHz

Time Weighting	Measured value (dB)	Deviated value (dB)	Uncertainty (dB)	Acceptance limit (dB)
Fast	94.0	0.0	0.20	±0.3
Slow	94.1	0.1	0.20	±0.3

Note: Time Weighting at 1 kHz are not accredited

4. Acoustical signal test of frequency weightings

A-Weighting acoustic frequency response meter free-field acoustic response at a level of 80.0 dB

Frequency Weighting (Hz)	Deviation from various frequency weighting response curve		
	A-Weighting (dB)	Uncertainty (dB)	Acceptance limit (dB)
125	0.0	0.20	±1.5
1000	-0.2	0.20	±1.0
8000	2.2	0.20	±5.0

Note: Acoustical signal test of frequency weightings are not accredited

Date of calibration : 2024-10-01
Date of Issue : 2024-10-02