

ภาคผนวกที่ 5
เอกสารสอบเทียบเครื่องมือตรวจวัด

ภาคผนวกที่ 5-1
เอกสารสอบเทียบเครื่องมือตรวจวัดคุณภาพอากาศ

CERTIFICATE OF CALIBRATION

Certificate No. : COF-017-67

Page 1 of 2 Pages

MEASUREMENT ITEM : Top Load Orifice
MANUFACTURER : TISCH
MODEL/TYPE : TE-5025A
SERIAL NUMBER : 710725
ID NUMBER : -
CONDITION AS-RECEIVED : Used item
CUSTOMER : Pacific Laboratory Co., Ltd.
14/5358 Moo14, T.Bang Bua Thong, A.Bang Bua Thong,
Nonthaburi 11110, Thailand.

RECEIVED DATE : 28 May 2024
MEASUREMENT DATE : 31 May 2024
ISSUE DATE : 31 May 2024

ENVIRONMENTAL CONDITIONS:

Ambient condition in the laboratory are as follow:

Temperature	: 23.0 ± 3.0	°C
Relative Humidity	: 55.0 ± 15.0	%RH
Atmospheric Pressure	: 1010 ± 10	hPa

CALIBRATION CONDITION:

Preconditioning : 24 hours at ambient conditions.
Measurement Condition : The average values during measurement are 23.1 °C and 50.4 %RH.

NOTED: The certificate is valid only to the item calibrated on date and place of calibration.

TABULATION OF RESULTS:

The table on next page give the measured values.

Calibration procedure:

The Orifice gas flow device was calibrated against Standard Rotary Displacement Meter (Roots Meter) Model G65/IMC/W2-dp. The WI-CL-004 was used as a calibration guideline.

Traceability:


This certificate provides a traceability of the measurement to recognized the national standards, and to realization of the international system of units (SI) through the NIMT (National Metrology Institute of Thailand) via Certificate number: MW-0063-23.

Uncertainty of Measurement:

The reported uncertainty of measurement is based on the standard uncertainty multiplied by a coverage factor $k=2$, Which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty has been determined in accordance with the GUM 'Evaluation of measurement data - Guide to the expression of uncertainty in measurement'

Calibrated by:

- ☒ Mr. Sorawit Thachalad
☐ Miss Jittraporn Lertsomphol

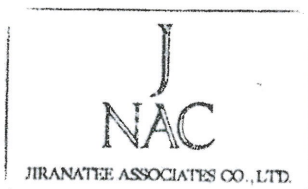

Approved signatory:

Mr. Parinya Booncharoen
Calibration Department Manager

MEASUREMENT RESULTS:

The Orifice gas flow device was calibrated by direct comparison method with the Standard Rotary Displacement Meter (Roots Meter). The Humid air was used as a medium in the system. The standard conditions are 25°C (298.15 K) and 760 mmHg for standard temperature and standard pressure respectively.

Table 1: The results of Q Standard calibration data

Plate	Flow rate m^3/min	Pressure [Pa] mmHg	Temperature [Ta] °C	Temperature [Tm] °C	Δp_{meter} mmHg	$\Delta p_{Orifice}$ inH ₂ O	γ	Standard Flow [Q_s] m^3/min
1	0.702	752.536	23.17	22.37	49.860	1.691	1.298	0.655
2	1.002	752.502	23.34	22.68	63.856	3.329	1.821	0.915
3	1.110	752.584	23.41	22.80	42.943	4.353	2.082	1.044
4	1.167	752.462	23.62	22.97	32.314	4.956	2.220	1.113
5	1.423	752.441	23.74	23.07	29.684	7.471	2.725	1.362


Slope (m): 2.01598
 Intercept (b): -0.02301
 Correlation coefficient (r): 0.99985
 Uncertainty ($k=2$): 0.015 m^3/min

Table 2: The results of Q actual calibration data

Plate	Flow rate m^3/min	Pressure [Pa] mmHg	Temperature [Ta] °C	Temperature [Tm] °C	Δp_{meter} mmHg	$\Delta p_{Orifice}$ inH ₂ O	γ	Standard Flow [Q_s] m^3/min
1	0.702	752.536	23.17	22.37	49.860	1.691	0.816	0.657
2	1.002	752.502	23.34	22.68	63.856	3.329	1.145	0.919
3	1.110	752.584	23.41	22.80	42.943	4.353	1.310	1.049
4	1.167	752.462	23.62	22.97	32.314	4.956	1.398	1.119
5	1.423	752.441	23.74	23.07	29.684	7.471	1.717	1.370

Slope (m): 1.26266
 Intercept (b): -0.01445
 Correlation coefficient (r): 0.99985
 Uncertainty ($k = 2$): 0.015 m^3/min

End of Certificate of Calibration

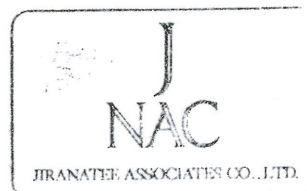

CALIBRATION TEST REPORT FOR Partisol Air Sampler

Calibrated Date: 22 September 2024

Report No: PM-202309022

Calibrated Due on: 21 September 2025

Instruments Information

Description : Thermo Scientific Partisol 2025i
Sequential Air Sampler

Model : 2025I

Sample flow control and reporting : 10 - 19 LPM

Serial No. : 2025I205851402

Environment : Temperature 25.5 °C

Instrument used for calibration [STD]

Description : Flow Meter

BIOS DryCal DC-Lite

Model : DCL-M REV. 1.08


Range : 200 ml/min - 20 L/min

Serial No. : 5016

Humidity: 51 %RH

Calibration Report

Filter	Set Flow Instrument (L/Min)	Current Flow Instrument reading (L/Min)	Actual Flow Reference standard (L/Min)	Error	Drift%
47 mm	15.00	15.00	14.99	-0.02	0.10
	16.67	16.67	16.66	-0.01	0.05
	18.34	18.34	18.31	-0.03	0.15

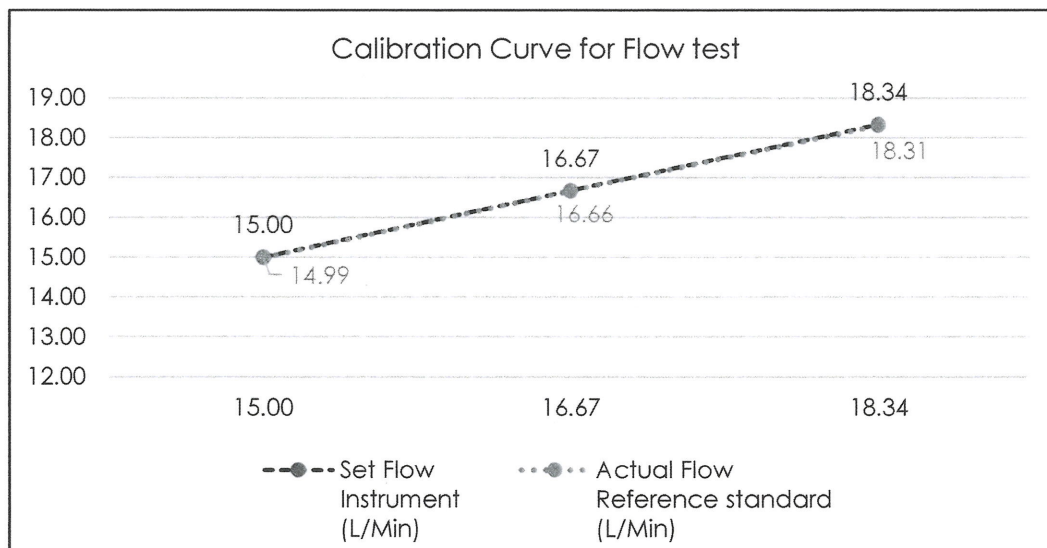

Calibrate By: กิตติศักดิ์ จันทะวงษ์

MR. KITTISAK JANSANGWATTANA

Approve by: MR. PASAGORN SAMOL

MR. PASAGORN SAMOL

CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhprachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech-cal@yahoo.com, calibratech-cal@hotmail.com



Certificate of Calibration

Certificate No. : 67-200273-1

Page : 1 of 2

Submitted by : Pacific Laboratory Co., Ltd.

14/5358 Moo 14, T.Bang Bua Thong, A.Bang Bua Thong, Nonthaburi 11110 Thailand

Equipment : Electronic Balance

Manufacturer : SHIMADZU

Model : AP225WD

Serial No. : D316301828

ID No. : LAB-BL-003

Capacity : 220000 mg

Resolution : 0.01mg/102000mg, 0.1mg/220000mg

Environment : On site calibration was carried out at the Laboratory, Pacific Laboratory Co., Ltd.

Ambient Temperature : (26.2 to 26.4) °C

Relative Humidity : (34.0 to 35.4) %

Air Pressure : 1007.0 mbar

Date of Received : 30 July 2024

Date of Calibration : 30 July 2024

Date of Issue : 31 July 2024

Calibrated by : Akaradath Thippichai

Calibration Method : In-house method CAL-M2001 based on UKAS Publication ref : LAB 14

Edition 7 - November 2022

Reference Standard Instruments : This certification is traceable to the International System of Units

Standard Weights

ID No.	Cert. No.	Due Date	Traceability
E261-E2624	C02232088	08 Nov 2024	National Institute of Metrology (Thailand), (NIMT)

Approved by :

(Surachai Promthong)

Laboratory Manager

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.

CAL-F0031-03



CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhprachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech_cal@yahoo.com, calibratech_cal@hotmail.com

Certificate of Calibration

Certificate No. : 67-200273-1

Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Departure of indication from nominal value

Nominal Value (mg)	Correction (mg)	Uncertainty \pm (mg)
1	0.01	0.012
10	0.01	0.012
50	0.01	0.012
100	0.01	0.014
1000	0.00	0.026
2000	0.01	0.034
5000	0.00	0.043
20000	0.00	0.071
50000	0.01	0.11
100000	0.00	0.20
150000	0.0	0.38
200000	0.0	0.38


This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2.06$, providing a level of confidence of approximately 95%

Eccentric error

Load test : 50000 mg

A	B	C	D	E	
0.00	0.00	0.01	0.00	0.00	mg



Repeatability

Load test : 200000 mg
Stdev. : 0.053 mg

Handwritten signature or initials.

- oOo -





บริษัท เอ็นไวร์ เซอร์วิส จำกัด

42 รามอินทรา 14 แขวง 9 เขตบางเขน กรุงเทพฯ 10230 โทรศัพท์ 02-9435814-5 โทรสาร 02-9438201
บริษัท เอ็นไวร์ เซอร์วิส จำกัด 42 Raminthra 14 yeak 9, Tha Rang, Bangkhen, Bankok 10230 Tel : 02-9435814-5 Fax : 02-9438201
ENVIR SERVICE CO., LTD.

Analyzer Performance Test

Calibrated Date: 7 August 2024

Instruments Information

Analyzer Type: SO2 Analyzer Model: 43C	Manufacturer Thermo Environmental S/N: 0607415772
---	--

Calibration System


Calibrator Unit	Standard Gas
Dilutor Model Dasibi Model 5008 S/N: 705 ZERO AIR Generator API MODEL 701 S/N: 1924	NO Conc 46.05 PPM SO2 Conc 46.01 PPM CO Conc 4,487 PPM Expire Date: 19 Sep. 2020

Environment: Temperature 25.5 °C

Humidity: 51 %RH

Calibration Report

Status	Zero			Span		
	Reference (PPB)	Reading (PPB)	Drift (PPB)	Reference (PPB)	Reading (PPB)	Drift%
Before	0.0	0.1	0.1	400.0	394.2	-1.5
After	0.0	0.0	0.0	400.0	400.0	0.0

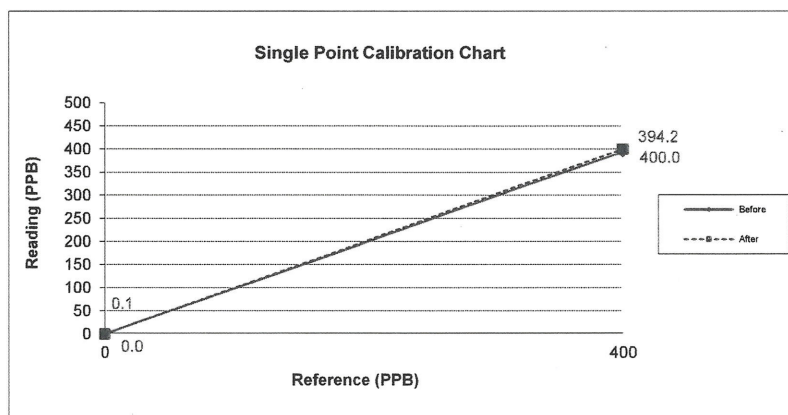

Calibrate By :

Mr.PASAGORN SAMOL



บริษัท เอ็นไวร์ เซอร์วิส จำกัด

42 รามอินทรา 14 แขวง 9 เขตบางเขน กรุงเทพมหานคร 10230 โทรศัพท์ 02-9435814-5 โทรสาร 02-9438201
บริษัท เอ็นไวร์ เซอร์วิส จำกัด
ENVIR SERVICE CO., LTD. 42 Raminthra 14 yeak 9, Tha Rang, Bangkhen, Bankok 10230 Tel : 02-9435814-5 Fax : 02-9438201

Analyzer Performance Test

Calibrated Date: 7 August 2024

Instruments Information

Analyzer Type: SO2 Analyzer Model: 43C	Manufacturer: Thermo Environmental S/N: 6067415770
---	---

Calibration System


Calibrator Unit	Standard Gas
Dilutor Model Dasibi Model 5008 S/N: 705 ZERO AIR Generator API MODEL 701 S/N: 1924	NO Conc 46.05 PPM SO2 Conc 46.01 PPM CO Conc 4,487 PPM Expire Date: 19 Sep. 2020

Environment: Temperature 25.5 °C

Humidity: 51 %RH

Calibration Report

Status	Zero			Span		
	Reference (PPB)	Reading (PPB)	Drift (PPB)	Reference (PPB)	Reading (PPB)	Drift%
Before	0.0	0.1	0.1	400.0	394.2	-1.5
After	0.0	0.0	0.0	400.0	400.0	0.0

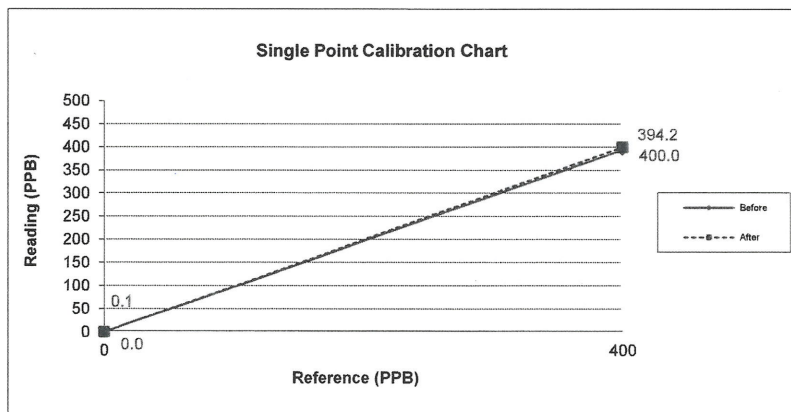

Calibrate By :

Mr.PASAGORN SAMOL



บริษัท เอ็นไวร์ เซอร์วิส จำกัด

42 รามอินทรา 14 แยก 9 แขวงท่าแร้ง เขตบางเขน กรุงเทพฯ 10230 โทรศัพท์ 02-9435814-5 โทรสาร 02-9438201
บริษัท เอ็นไวร์ เซอร์วิส จำกัด
ENVIR SERVICE CO., LTD. 42 Raminthra 14 yeak 9, Tha Rang, Bangkhen, Bankok 10230 Tel : 02-9435814-5 Fax : 02-9438201

Analyzer Performance Test

Calibrated Date: 9 August 2024

Instruments Information

Analyzer Type: NO/NO ₂ /NO _x Analyzer Model: 42C	Manufacturer Thermo Environmental S/N: 42C-63476-339
---	---

Calibration System

Calibrator Unit	Standard Gas
Dilutor Model Dasibi Model 5008 S/N: 705 ZERO AIR Generator API Model 701 S/N: 1924	NO Conc 46.05 PPM SO ₂ Conc 46.01 PPM CO Conc 4.487 PPM Expire Date: 19 Sep. 2020

Environment: Temperature 25.5 °C


Humidity: 51 %RH

Calibration Check (Before adjust)

GAS	Zero			Span		
	Reading Value (ppb)	Expected Value (ppb)	Drift (ppb)	Reading Value (ppb)	Expected Value (ppb)	Drift%
NO	0.1	0.0	0.1	397.7	400.0	-0.6
NO _x	0.1	0.0	0.1	400.0	400.0	0.0

Calibration Check (After adjust)

GAS	Zero			Span		
	Reading Value (ppb)	Expected Value (ppb)	Drift (ppb)	Reading Value (ppb)	Expected Value (ppb)	Drift%
NO	0.0	0.0	0.0	400.0	400.0	0.0
NO _x	0.0	0.0	0.0	400.0	400.0	0.0

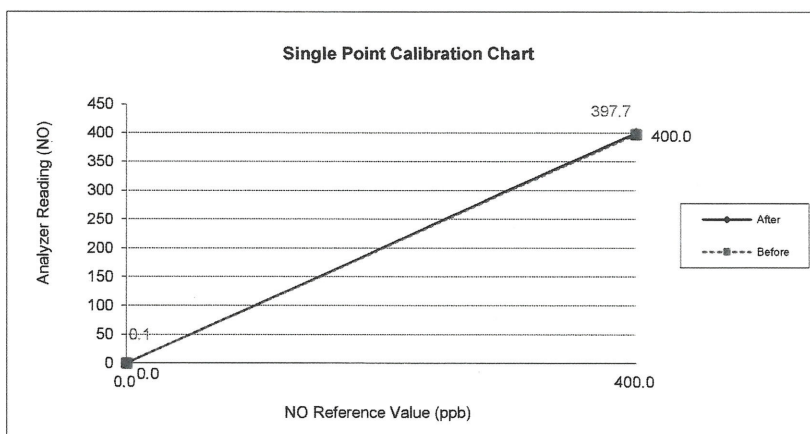

Calibrate By : Mr. Pasagorn Samol



บริษัท เอ็นไวร์ เซอร์วิส จำกัด

42 รามอินทรา 14 แยก 9 แขวงท่าแร้ง เขตบางเขน กรุงเทพฯ 10230 โทรศัพท์ 02-9435814-5 โทรสาร 02-9438201
บริษัท เอ็นไวร์ เซอร์วิส จำกัด
ENVIR SERVICE CO., LTD. 42 Raminthra 14 yeak 9, Tha Rang, Bangkhen, Bankok 10230 Tel : 02-9435814-5 Fax : 02-9438201

Analyzer Performance Test

Calibrated Date: 9 August 2024

Instruments Information

Analyzer Type: NO/NO ₂ /NO _x Analyzer Model: 42C	Manufacturer Thermo Environmental S/N: 65850-350
---	---

Calibration System

Calibrator Unit	Standard Gas
Dilutor Model Dasibi Model 5008 S/N: 705 ZERO AIR Generator API Model 701 S/N: 1924	NO Conc 46.05 PPM SO ₂ Conc 46.01 PPM CO Conc 4.487 PPM Expire Date: 19 Sep. 2020

Environment: Temperature 25.5 °C


Humidity: 51 %RH

Calibration Check (Before adjust)

GAS	Zero			Span		
	Reading Value (ppb)	Expected Value (ppb)	Drift (ppb)	Reading Value (ppb)	Expected Value (ppb)	Drift%
NO	0.1	0.0	0.1	397.2	400.0	-0.7
NO _x	0.1	0.0	0.1	400.0	400.0	0.0

Calibration Check (After adjust)

GAS	Zero			Span		
	Reading Value (ppb)	Expected Value (ppb)	Drift (ppb)	Reading Value (ppb)	Expected Value (ppb)	Drift%
NO	0.0	0.0	0.0	400.0	400.0	0.0
NO _x	0.0	0.0	0.0	400.0	400.0	0.0

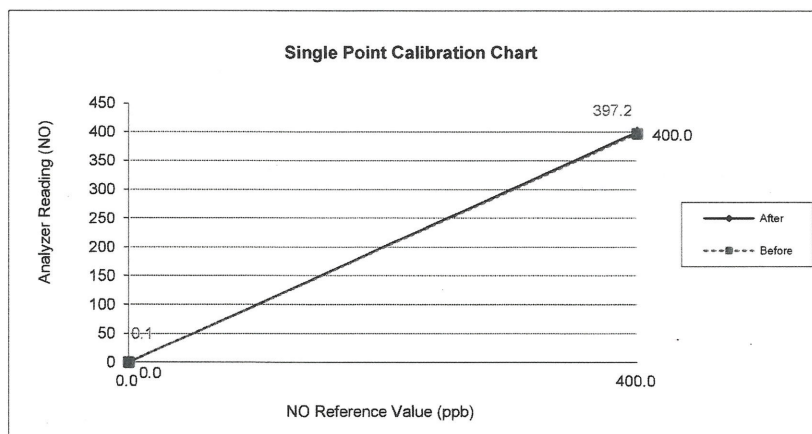

Signature

Calibrate By : Mr. Pasagorn Samol



บริษัท เอ็นไวร์ เซอร์วิส จำกัด

42 รามอินทรา 14 แยก 9 แขวงท่าแร้ง เขตบางเขน กรุงเทพฯ 10230 โทรศัพท์ 02-9435814-5 โทรสาร 02-9438201
บริษัท เอ็นไวร์ เซอร์วิส จำกัด
ENVIR SERVICE CO., LTD. 42 Raminthra 14 yeak 9, Tha Rang, Bangkhen, Bankok 10230 Tel : 02-9435814-5 Fax : 02-9438201

Analyzer Performance Test

Calibrated Date: 11 August 2024

Instruments Information

Analyzer Type: CO Analyzer Model: 48C	Manufacturer: Thermo Environmental S/N: 48C-0604815184
--	---

Calibration System


Calibrator Unit	Standard Gas
Dilutor Model Dasibi Model 5008 S/N: 705 ZERO AIR Generator API MODEL 701 S/N: 1924	NO Conc 46.05 PPM SO2 Conc 46.01 PPM CO Conc 4,487 PPM Cylinder number CC507080 Expire Date: 19 Sep. 2020

Environment: Temperature 25.5 °C

Humidity: 51 %RH

Calibration Report

Status	Zero			Span		
	Reference (PPM)	Reading (PPM)	Drift (PPM)	Reference (PPM)	Reading (PPM)	Drift%
Before	0.0	0.1	0.1	45.0	44.2	-1.8
After	0.0	0.0	0.0	45.0	45.0	0.0

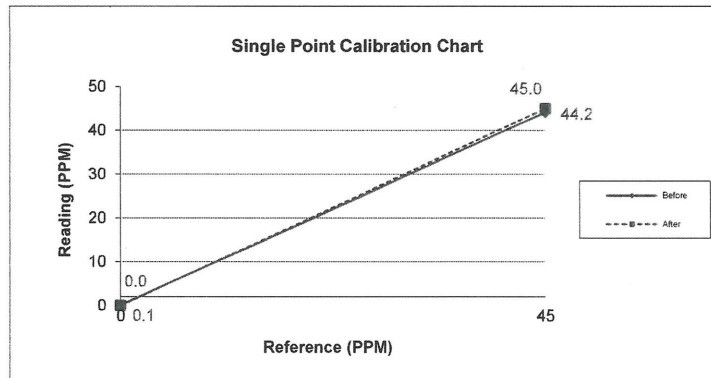

Calibrate By :

Mr. PASAGORN SAMOL



บริษัท เอ็นไวร์ เซอร์วิส จำกัด

42 รามอินทรา 14 แยก 9 แขวงท่าแร้ง เขตบางเขน กรุงเทพมหานคร 10230 โทรศัพท์ 02-9435814-5 โทรสาร 02-9438201
บริษัท เอ็นไวร์ เซอร์วิส จำกัด
ENVIR SERVICE CO., LTD. 42 Raminthra 14 yeak 9, Tha Rang, Bangkhen, Bankok 10230 Tel : 02-9435814-5 Fax : 02-9438201

Analyzer Performance Test

Calibrated Date: 11 August 2024

Instruments Information

Analyzer Type: CO Analyzer Model: 48C	Manufacturer Thermo Environmental S/N: 0514811738
--	--

Calibration System


Calibrator Unit	Standard Gas
Dilutor Model Dasibi Model 5008 S/N: 705 ZERO AIR Generator API MODEL 701 S/N: 1924	NO Conc 46.05 PPM SO2 Conc 46.01 PPM CO Conc 4.487 PPM Expire Date: 19 Sep. 2020

Environment: Temperature 25.5 °C

Humidity: 51 %RH

Calibration Report

Status	Zero			Span		
	Reference (PPM)	Reading (PPM)	Drift (PPM)	Reference (PPM)	Reading (PPM)	Drift%
Before	0.0	0.1	0.1	45.0	44.5	-1.1
After	0.0	0.0	0.0	45.0	45.0	0.0

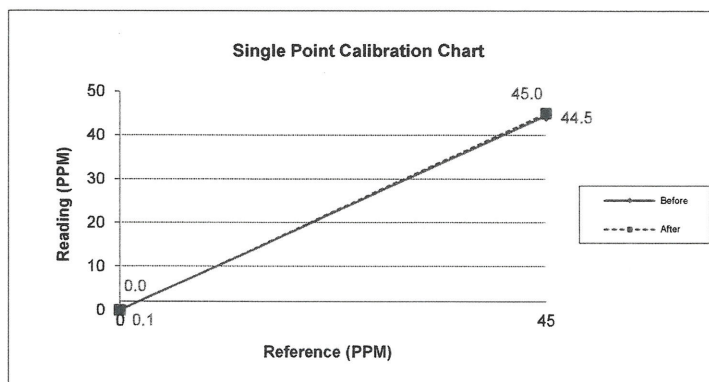

Calibrate By :

Mr. PASAGORN SAMOL

Analyzer Performance Test

Calibrated Date: 24 April 2024

Instruments Information

Analyzer Type : Methane-NMHC Analyzer
Model : 55C

Manufacturer : Thermo Environmental
Serial Number : 55C-0515611965

Calibrator Unit

Dilutor Model : Dasibi Model 5008
Serial Number : 705
ZERO AIR Generator : API MODEL 701
Serial Number : 1924

Standard Gas Concentration

Methane (CH₄) 183.0 PPM
Propane 59.1 PPM
Cylinder number 4860
Expire Date: 6 Dec. 2025


Environment : Temperature 25.5 °C Humidity: 51 %RH

Calibration Report (Before adjust)

Status	Zero			Span		
	Reference (PPM)	Reading (PPM)	Drift (PPM)	Reference (PPM)	Reading (PPM)	Drift%
Methane	0.0	0.1	0.1	183.0	181.2	-1.0
NMHC	0.0	0.1	0.1	59.1	58.3	-1.4

Calibration Report (After adjust)

Status	Zero			Span		
	Reference (PPM)	Reading (PPM)	Drift (PPM)	Reference (PPM)	Reading (PPM)	Drift%
Methane	0.0	0.0	0.0	183.0	182.7	-0.2
NMHC	0.0	0.0	0.0	59.1	59.0	-0.2

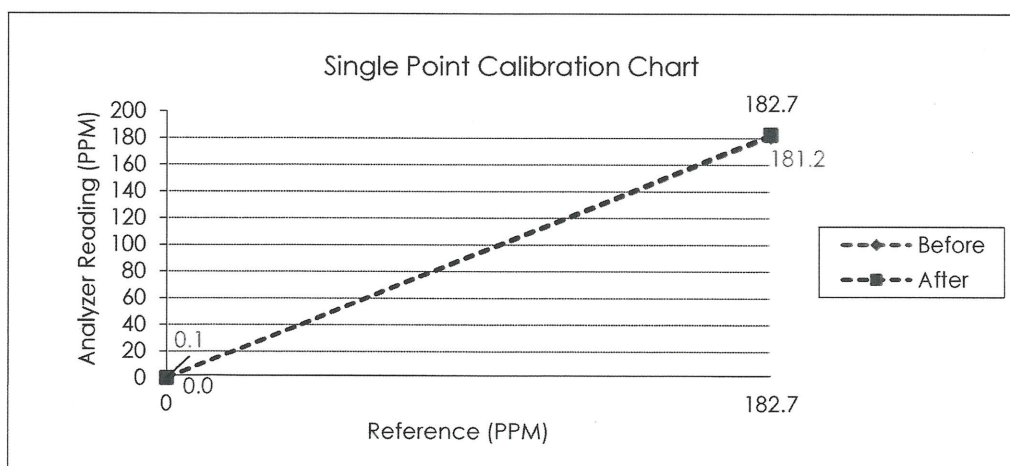

Calibrate By : 
MR. KITTISAK JANSANGWATTANA

Approve by : 
MR. PASAGORN SAMOL

ภาคผนวกที่ 5-2
เอกสารสอบเทียบเครื่องมือตรวจวัดระดับเสียง




Professional Calibration & Services Co., Ltd.

50/888, 50/889 Moo 2, Rungsit-Nakornnayok Rd., Bungyeetho, Thunyaburi,
Pathumthani 12130 Thailand

Tel : (+66)2150-6641 (Autoline), (+66)2569-5158

Email : info@p-cal.com www.p-cal.com



Certificate of Calibration

Certificate Number : EL41650/24

Page 1 of 3

Control Number : PCAL153035

Customer Control : -

Description : Sound Calibrator

Manufacturer : SOUNDTEK

Model : ST-120

Serial Number : 211203764

Customer : Pacific Laboratory Co., Ltd.

14/5358 Moo 14, Tambol Bang Bua Thong, Amphoe Bang Bua Thong,
Nonthaburi 11110


Date of Receipt : 22-Aug-24

Date of Calibration : 23-Aug-24

Environment : Temperature $23^{\circ}\text{C} \pm 2^{\circ}\text{C}$
: Relative Humidity $50\% \pm 20\%$

Calibration Method : Calibration Procedure Number CP-EL35

Calibration Results : See data attached



The reported uncertainty is based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%.

This certificate is issued in accordance with ISO/IEC17025 and the conditions of accreditation granted by the Accreditation Body which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory. The results relate only to the item calibrated.

This certificate shall not be reproduced other than in full except without the prior written approval of the Head of Calibration Laboratory of Professional Calibration & Services Co., Ltd.

Calibrated By

Mr. Nonpawit Wiseshoo

Authorized Signature

(Mr. Manote Piwnimnual)

27-Aug-24

Issued Date

CALIBRATION REPORT

Professional Calibration & Services Co.,Ltd.

Certificate Number : EL41650/24

Page 2 of 3

Equipment Standards Used

Description	Serial No.	Traceability to	Certificate No.	Cal. Due Date
Sound Level Meter	030606101	ANAB : AC-2590	EL12298/24	27-Mar-25
Sound Calibrator	125626778	NSC : Calibration 0037	EEL.BP. 161/0167	04-Feb-25

Condition as received : Normal

Definitions :-

- * ANAB - The ANSI National Accreditation Board
- * NSC - National Standardization Council of Thailand

CALIBRATION REPORT

Professional Calibration & Services Co., Ltd.

Certificate No.: EL41650/24


Page : 3 of 3

Calibration Results

Sound Pressure Level Accuracy


Nominal Value	Measured Value	UUC Error	Uncertainty (±)
94 dB	93.97 dB	0.03 dB	0.17 dB
114 dB	114.30 dB	-0.30 dB	0.17 dB

...End...



APTITECH CALIBRATION CO., LTD.

50/40 Moo 5 T. Lat Sawai, A. Lamlukka, Pathumthani 12150
Tel. +66 2103-6290 Fax. +66 2103-6291
Email. sales@aptitech-cal.com



CERTIFICATE OF CALIBRATION

Certificate Number : SC240209

Customer : Pacific Laboratory Co.,Ltd.
Address : 14/5358 Moo 14 Tambol Bang Bua Thong, Amphoe Bang Thong,
Nonthaburi 11110

Description	: Sound Level Meter	W/O Number	: SC240209
Manufacturer	: Scarlet Tech	Calibration Location	: Laboratory
Model	: ST-11D	Ambient Temperature	: 22 ± 2 °C
Serial Number	: 820968	Ambient Humidity	: 55 ± 15 %RH
ID. Number	: N/A	Received Date	: 20-Aug-2024

This certifies that the above instrument was calibrated in compliance with the Calibration Systems Requirement of ISO/IEC 17025:2017 in accordance with referenced procedures. Standards used to perform this calibration are certified by or traceable to National Institute of Metrology (Thailand) and/or other recognized national measurement institutes which realizes the units of measurement according to the International System of Units (SI Unit).

Measurement uncertainties at the time of test are given where applicable. They are calculated in accordance with the method described in The Expression of Uncertainty and Confidence in Measurement (M3003).

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by coverage factor $k=2$ such that the coverage probability corresponds to approximately 95%. This result of calibration was found accurate as shown on date and place of calibration only.

Standard Equipments

Description	Serial No.	Certificate No.	Traceability	Due Date
Sound Level Calibrator	141011576	CP20240179EA	TISI: 22-LB0119	14-May-25



Authority of Calibration

Approved Signatory

☒ Mr. Anuwat Simsiriwat [Laboratory Manager]


☐ Mr. Nattaphol Boonmee [Quality Manager]

Calibration Date : 21-Aug-2024

Issued Date : 24-Aug-2024

Calibrated By : Ms. Hathaichanok Kaewsrisai

Calibration certificates without signatures are not valid. This certificate applied to only the item identified and shall not be reproduced other than in full, without the specific written approval by APTITECH CALIBRATION CO., LTD.




APTITECH CALIBRATION CO., LTD.

50/40 Moo 5 T. Lat Sawai, A. Lamukha, Pathumthani 12150

Tel. +66 2103-6290 Fax. +66 2103-6291

Email: sales@aptitech-cal.com



CALIBRATION REPORT

Certificate Number : SC240209

Calibration Method

The Unit Under Calibration (UUC) was calibrated by comparison measurement with sound level calibrator. The calibration has been accomplished in an ambient environment controlled, base on the in-house calibration procedure. The identification of the laboratory's calibration procedure employed are CP-7.2-01-107

Calibration Results

Appearance and function of use : Good
Results of Calibration : Without any adjustment
Sound Level Calibration
- Frequency Weighting : A
- Resolution : 0.1 dB


Sound Level Measurement (Slow Mode)

Parameter	UUC Range	Standard Value	UUC Reading	UUC Error	(±) Uncertainty
LFp	20-140 dB	93.86 dB	93.6 dB	-0.26 dB	0.60 dB
		113.87 dB	113.6 dB	-0.27 dB	0.60 dB
LSp	20-140 dB	93.86 dB	93.6 dB	-0.26 dB	0.60 dB
		113.87 dB	113.6 dB	-0.27 dB	0.60 dB
LIp	20-140 dB	93.86 dB	93.6 dB	-0.26 dB	0.60 dB
		113.87 dB	113.6 dB	-0.27 dB	0.60 dB

Sound Level Measurement (Fast Mode)

Parameter	UUC Range	Standard Value	UUC Reading	UUC Error	(±) Uncertainty
LFp	20-140 dB	93.86 dB	93.6 dB	-0.26 dB	0.60 dB
		113.87 dB	113.5 dB	-0.37 dB	0.60 dB
LSp	20-140 dB	93.86 dB	93.6 dB	-0.26 dB	0.60 dB
		113.87 dB	113.5 dB	-0.37 dB	0.60 dB
LIp	20-140 dB	93.86 dB	93.6 dB	-0.26 dB	0.60 dB
		113.87 dB	113.5 dB	-0.37 dB	0.60 dB

--- End of Certificate ---




APTITECH CALIBRATION CO., LTD.

50/40 Moo 5 T. Lat Sawai, A. Lam Lukka, Pathumthani 12150

Tel. +66 2103-6290 Fax. +66 2103-6291

Email. sales@aptitech-cal.com



CERTIFICATE OF CALIBRATION

Certificate Number : SC240093

Customer : Pacific Laboratory Co.,Ltd.
Address : 14/5358 Moo 14 Tambol Bang Bua Thong, Amphoe Bang Thong,
Nonthaburi 11110

Description	: Sound Level Meter	W/O Number	: SC240093
Manufacturer	: Scarlet Tech	Calibration Location	: Laboratory
Model	: ST-11D	Ambient Temperature	: 22 ± 2 °C
Serial Number	: 820967	Ambient Humidity	: 55 ± 15 %RH
ID. Number	: N/A	Received Date	: 23-Mar-2024

This certifies that the above instrument was calibrated in compliance with the Calibration Systems Requirement of ISO/IEC 17025:2017 in accordance with referenced procedures. Standards used to perform this calibration are certified by or traceable to National Institute of Metrology (Thailand) and/or other recognized national measurement institutes which realizes the units of measurement according to the International System of Units (SI Unit).

Measurement uncertainties at the time of test are given where applicable. They are calculated in accordance with the method described in The Expression of Uncertainty and Confidence in Measurement (M3003).

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by coverage factor $k=2$ such that the coverage probability corresponds to approximately 95%. This result of calibration was found accurate as shown on date and place of calibration only.

Standard Equipments

Description	Serial No.	Certificate No.	Traceability	Due Date
Sound Level Calibrator	141011576	CP20230261EA	TISI: 22-LB0119	05-Jul-24



Authority of Calibration

Approved Signatory

Calibration Date : 23-Mar-2024


Issued Date : 26-Mar-2024

Calibrated By : Ms. Hathaichanok Kaewsrisai

☐ Mr. Anuwat Simsiriwat [Laboratory Manager]

☒ Mr. Sompoch Srisunart [Technical Manager]

Calibration certificates without signatures are not valid. This certificate applied to only the item identified and shall not be reproduced other than in full, without the specific written approval by APTITECH CALIBRATION CO., LTD.




APTITECH CALIBRATION CO., LTD.

50/40 Moo 5 T. Lat Sawai, A. Lamukha, Pathumthani 12150

Tel. +66 2103-6290 Fax. +66 2103-6291

Email. sales@aptitech-cal.com



CALIBRATION REPORT

Certificate Number : SC240093

Calibration Method

The Unit Under Calibration (UUC) was calibrated by comparison measurement with sound level calibrator. The calibration has been accomplished in an ambient environment controlled, base on the in-house calibration procedure. The identification of the laboratory's calibration procedure employed are CP-7.2-01-107

Calibration Results

Appearance and function of use : Good
Results of Calibration : Without any adjustment
Sound Level Calibration
- Frequency Weighting : A
- Resolution : 0.1 dB

Sound Level Measurement (Slow Mode)

Parameter	UUC Range	Standard Value	UUC Reading	UUC Error	(±) Uncertainty
LFp	20-140 dB	93.86 dB	93.7 dB	-0.16 dB	0.61 dB
		113.87 dB	113.7 dB	-0.17 dB	0.61 dB
LSp	20-140 dB	93.86 dB	93.7 dB	-0.16 dB	0.61 dB
		113.87 dB	113.7 dB	-0.17 dB	0.61 dB
LIp	20-140 dB	93.86 dB	93.7 dB	-0.16 dB	0.61 dB
		113.87 dB	113.7 dB	-0.17 dB	0.61 dB

Sound Level Measurement (Fast Mode)

Parameter	UUC Range	Standard Value	UUC Reading	UUC Error	(±) Uncertainty
LFp	20-140 dB	93.86 dB	93.7 dB	-0.16 dB	0.61 dB
		113.87 dB	113.8 dB	-0.07 dB	0.61 dB
LSp	20-140 dB	93.86 dB	93.7 dB	-0.16 dB	0.61 dB
		113.87 dB	113.8 dB	-0.07 dB	0.61 dB
LIp	20-140 dB	93.86 dB	93.7 dB	-0.16 dB	0.61 dB
		113.87 dB	113.8 dB	-0.07 dB	0.61 dB

--- End of Certificate ---


ภาคผนวกที่ 5-3
เอกสารสอบเทียบเครื่องมือตรวจวัดความสั่นสะเทือน



CLC
Accredited
ISO/IEC 17025

CALIBRATION LABORATORY Co., LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



CERTIFICATE OF CALIBRATION

FOR

NOMENCLATURE : VIBRATION METER
MANUFACTURER : INSTANTEL
MODEL / TYPE : 721A2501/721A2901
SERIAL NO. : UM13202/UM13202
CLID. NO. : 252102517
JOB CONTROL NO. : 240125008596
CALIBRATION SERVICE : ☒ IN-LABORATORY ☐ ON-SITE

CUSTOMER : PACIFIC LABORATORY CO., LTD.
14/5358 MOO 14 TAMBOL BANG BUA THONG
AMPHOE BANG BUA THONG NONTABURI 11110


DATE OF RECEIVED : 25 January 2024

DATE OF ISSUED : 30 January 2024

The report of calibration shall not be reproduced except in full without approval of the Calibration Laboratory Co., Ltd.

Calibrated By :

Suwit Phuanbusabong
Calibration Engineer



Approved By :

Mongkol Yotsoontorn
Authorized Signatory

30 January 2024

This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to the International System of Units (SI)

Certificate No. Q24008596

F3-011-05/12-23

page 1 of 2



@clccalibrat




CLC
Accredited
ISO/IEC 17025

CALIBRATION LABORATORY Co., LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230

Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



REPORT OF CALIBRATION FOR

NOMENCLATURE	:	VIBRATION METER
MANUFACTURER	:	INSTANTEL
MODEL / TYPE	:	721A2501/721A2901
SERIAL NO.	:	UM13202/UM13202
DATE OF CALIBRATION	:	26 January 2024

ENVIRONMENT CONDITIONS :

Temperature : $(23 \pm 2) ^\circ\text{C}$

Relative Humidity : $(55 \pm 15) \% \text{RH}$

PROCEDURE USED :

This instrument was calibrated under procedure No. **CLC-CPEE-08** based on **ISO 16063-21** as calibration guideline.

The calibration was performed by using Digital Multimeter, Programmable Timer/Counter, Accelerometer and Measuring Amplifier which maintained by the Calibration Laboratory Co., Ltd.

REFERENCE STANDARD USED :

1. Digital Multimeter, Hewlett Packard Model 34401A S/N. US36044686.
2. Programmable Timer/Counter, Philips Model PM6680B S/N. SM607101.
3. Accelerometer with Measuring Amplifier, Bruel & Kjaer Model 8305, 2525 S/N. 397018, 2434988.

TRACEABILITY :

1. The measurements are traceable to International System of Units (SI), through National Institute of Metrology (Thailand) Certificate No. EE-0100-23, Due Date 01 December 2024.
2. The measurements are traceable to International System of Units (SI), through Aeronautical Radio of Thailand Ltd. Certificate No. 07-0043/23 , Due Date 12 April 2024.
3. The measurements are traceable to International System of Units (SI), through National Institute of Metrology (Thailand) Certificate No. AV-0052-23, Due Date 26 September 2024.

UNCERTAINTY :

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor $k = 2,00$ which for a normal distribution corresponds to a coverage probability of approximately 95 %.

It has been evaluated according to the "Evaluation of the Uncertainty of Measurement in Calibration (EA-4/02 M:2022)"

Certificate No. Q24008596

F3-011-05/12-23

page 2 of 3



@clccalibrat




CLC
Accredited
ISO/IEC 17025

CALIBRATION LABORATORY Co., LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230

Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



CONDITION OF CALIBRATION ITEM : RECEIVED IN GOOD OPERATIONAL CONDITION

MEASUREMENT RESULTS : (X) without adjustment () adjustment

CALIBRATION DATA

VELOCITY RESULT

Test point		Mode	STD Reading	DUC Reading	Correction	Uncertainty
(mm/s)	(frequency)		(mm/s)	(mm/s)	(mm/s)	± (% of rdg.)
10.0	160 Hz	peak	10.000	10.304	-0.304	1.1
20.0	160 Hz		20.000	20.396	-0.396	0.9
30.0	160 Hz		30.000	30.479	-0.479	0.9
40.0	160 Hz		40.000	40.587	-0.587	0.9
50.0	160 Hz		50.000	50.649	-0.649	0.9

Note. The Scope of Accredited ANAB Certificate No. ACDM-2814 Version 012 Page 2 of 67

This report is valid for the above stated instrument/s only.

End of Certificate

Certificate No. Q24008596

F3-011-05/12-23

page 3 of 3




@clccalibrati



CALIBRATION LABORATORY Co., LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



CERTIFICATE OF CALIBRATION

FOR

NOMENCLATURE : VIBRATION METER
MANUFACTURER : INSTANTEL
MODEL / TYPE : 721A2501/721A2901
SERIAL NO. : UM13203/UM13203
CLID. NO. : 252000160
JOB CONTROL NO. : 240125008595
CALIBRATION SERVICE : ☒ IN-LABORATORY ☐ ON-SITE

CUSTOMER : PACIFIC LABORATORY CO., LTD.
14/5358 MOO 14 TAMBOL BANG BUA THONG
AMPHOE BANG BUA THONG NONTABURI 11110


DATE OF RECEIVED : 25 January 2024

DATE OF ISSUED : 30 January 2024

The report of calibration shall not be reproduced except in full without approval of the Calibration Laboratory Co., Ltd.

Calibrated By :

Suwit Phuanbusabong
Calibration Engineer



Approved By :

Mongkol Yotsoontorn
Authorized Signatory

30 January 2024

This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to the International System of Units (SI)

Certificate No. Q24008595

F3-011-05/12-23

page 1 of 2




@clccalibrat



CALIBRATION LABORATORY Co., LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230

Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



REPORT OF CALIBRATION FOR

NOMENCLATURE	:	VIBRATION METER
MANUFACTURER	:	INSTANTEL
MODEL / TYPE	:	721A2501/721A2901
SERIAL NO.	:	UM13203/UM13203
DATE OF CALIBRATION	:	26 January 2024

ENVIRONMENT CONDITIONS :

Temperature : $(23 \pm 2) ^\circ\text{C}$

Relative Humidity : $(55 \pm 15) \% \text{RH}$

PROCEDURE USED :

This instrument was calibrated under procedure No. **CLC-CPEE-08** based on **ISO 16063-21** as calibration guideline.
The calibration was performed by using Digital Multimeter, Programmable Timer/Counter,
Accelerometer and Measuring Amplifier which maintained by the Calibration Laboratory Co., Ltd.

REFERENCE STANDARD USED :

1. Digital Multimeter, Hewlett Packard Model 34401A S/N. US36044686.
2. Programmable Timer/Counter, Philips Model PM6680B S/N. SM607101.
3. Accelerometer with Measuring Amplifier, Bruel & Kjaer Model 8305, 2525 S/N. 397018, 2434988.

TRACEABILITY :

1. The measurements are traceable to International System of Units (SI), through National Institute of Metrology (Thailand) Certificate No. EE-0100-23, Due Date 01 December 2024.
2. The measurements are traceable to International System of Units (SI), through Aeronautical Radio of Thailand Ltd. Certificate No. 07-0043/23, Due Date 12 April 2024.
3. The measurements are traceable to International System of Units (SI), through National Institute of Metrology (Thailand) Certificate No. AV-0052-23, Due Date 26 September 2024.

UNCERTAINTY :

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor $k = 2,00$ which for a normal distribution corresponds to a coverage probability of approximately 95 %.
It has been evaluated according to the "Evaluation of the Uncertainty of Measurement in Calibration (EA-4/02 M:2022)"

Certificate No. Q24008595

F3-011-05/12-23

page 2 of 3



@clccalibrat

CONDITION OF CALIBRATION ITEM : RECEIVED IN GOOD OPERATIONAL CONDITION

MEASUREMENT RESULTS : (X) without adjustment () adjustment

CALIBRATION DATA

VELOCITY RESULT

Test point		Mode	STD Reading	DUC Reading	Correction	Uncertainty
(mm/s)	(frequency)		(mm/s)	(mm/s)	(mm/s)	± (% of rdg.)
10.0	160 Hz	peak	10.000	10.234	-0.234	1.1
20.0	160 Hz		20.000	20.341	-0.341	0.9
30.0	160 Hz		30.000	30.446	-0.446	0.9
40.0	160 Hz		40.000	40.576	-0.576	0.9
50.0	160 Hz		50.000	50.613	-0.613	0.9

Note. The Scope of Accredited ANAB Certificate No. ACDM-2814 Version 012 Page 2 of 67

This report is valid for the above stated instrument/s only.

End of Certificate

Certificate No. Q24008595

F3-011-05/12-23

page 3 of 3



@clccalibrat

ภาคผนวกที่ 5-4
เอกสารสอบเทียบเครื่องมือตรวจวัดคุณภาพน้ำ

Certificate of Calibration

Certificate No. : 67-420078-1

Page : 1 of 2

Submitted by : Pacific Laboratory Co., Ltd.

14/5358 Moo 14, T. Bang Bua Thong, A. Bang Bua Thong, Nonthaburi 11110 Thailand

Equipment : pH Meter with electrode

pH meter

Manufacturer : Eutech

Model : pH 700

Range : N/A pH

Resolution : 0.01 pH

Serial No. : 2841305

ID No. : LAB-PH-002

Electrode

Model : N/A

Serial No. : 3172493

Environment : On site calibration was carried out at the Laboratory, Pacific Laboratory Co., Ltd

Ambient Temperature : (25.0 to 26.0) °C

Relative Humidity : (40 to 45) %

Date of Received : 30 July 2024

Date of Calibration : 30 July 2024

Date of Issue : 03 August 2024

Calibrated by : Permpon Chanpu

Calibration Method : In-house method CAL-M4201 direct measurement by using standard voltage calibrator and using certified reference material (CRM)

Reference Standard Instruments : This certification is traceable to the International System of Units

1. Multiproduct Calibrator

ID No.	Cert. No.	Due Date	Traceability
400005	SG-E-00307/66	23 Aug 2025	National Institute of Metrology Thailand (NIMT)

2. Standard Buffer Solution

pH	Cert. No.	Lot No.	Exp. Date	Traceability
4.008	61293328	986281	25 Apr 2026	CPA Chem Ltd. Accredited to ISO 17034 and ISO/IEC 17025
6.986	61281486	986283	25 Apr 2025	CPA Chem Ltd. Accredited to ISO 17034 and ISO/IEC 17025
9.997	61281073	986282	25 Apr 2025	CPA Chem Ltd. Accredited to ISO 17034 and ISO/IEC 17025

Approved by :

(Surachai Promthong)

Laboratory Manager

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhaprachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech.cal@yahoo.com, calibratech.cal@hotmail.com

Certificate of Calibration

Certificate No. : 67-420078-1

Page : 2 of 2

Result of Calibration :

UUC Condition As-Received : Good

Function : Electrical measurement

pH meter

Performing standard curve by Multiproduct Calibrator at pH (4,7,10)

Adjustment Curve at nominal pH	Applied Voltage (mV)	Nominal Value (pH)	UUC Reading		Correction (mV)	Uncertainty (± mV)
			(pH)	(mV)		
4, 7, 10	177.4800	4	4.00	177.5	0.0	0.12
	0.0000	7	7.00	0.1	-0.1	0.086
	-177.4800	10	10.00	-177.4	-0.1	0.12

Function : pH meter with electrode

Performing a three - buffer standard curve using buffer nominal pH (4,7,10)

Adjustment Curve at nominal pH	Standard Buffer (pH)	UUC Reading (pH)	Correction (pH)	Uncertainty (± pH)
4, 7, 10	4.008	4.01	0.00	0.0097
	6.986	7.00	-0.01	0.011
	9.997	10.01	-0.01	0.014

Remark

UUC : Unit Under Calibration

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

- 000 -



CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhprachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech.cal@yahoo.com, calibratech.cal@hotmail.com



NSC-TISI-TIS 17025
CALIBRATION 0030

Certificate of Calibration

Certificate No. : 67-420078-2

Page : 1 of 2

Submitted by : Pacific Laboratory Co., Ltd.

14/5358 Moo 14, T. Bang Bua Thong, A. Bang Bua Thong, Nonthaburi 11110 Thailand

Equipment : pH Meter with electrode

pH meter

Manufacturer : Eutech

Model : pH 700

Range : N/A

pH

Resolution : 0.01 pH

Serial No. : 2841305

ID No. : LAB-PH-002

Electrode

Model : N/A

Serial No. : 3052953

Environment : On site calibration was carried out at the Laboratory, Pacific Laboratory Co., Ltd

Ambient Temperature : (25.0 to 26.0)° C

Relative Humidity : (40 to 45) %

Date of Received : 30 July 2024

Date of Calibration : 30 July 2024

Date of Issue : 03 August 2024

Calibrated by : Permpon Chanpu

Calibration Method : In-house method CAL-M4201 direct measurement by using standard voltage calibrator and using certified reference material (CRM)

Reference Standard Instruments : This certification is traceable to the International System of Units

1. Multiproduct Calibrator

<u>ID No.</u>	<u>Cert. No.</u>	<u>Due Date</u>	<u>Traceability</u>
400005	SG-E-00307/66	23 Aug 2025	National Institute of Metrology Thailand (NIMT)

2. Standard Buffer Solution

<u>pH</u>	<u>Cert. No.</u>	<u>Lot No.</u>	<u>Exp. Date</u>	<u>Traceability</u>
4.008	61293328	986281	25 Apr 2026	CPA Chem Ltd. Accredited to ISO 17034 and ISO/IEC 17025
6.986	61281486	986283	25 Apr 2025	CPA Chem Ltd. Accredited to ISO 17034 and ISO/IEC 17025
9.997	61281073	986282	25 Apr 2025	CPA Chem Ltd. Accredited to ISO 17034 and ISO/IEC 17025

Approved by :

(Surachai Promthong)

Laboratory Manager

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 67-420078-2

Page : 2 of 2

Result of Calibration :

UUC Condition As-Received : Good

Function : Electrical measurement

pH meter

Performing standard curve by Multiproduct Calibrator at pH (4,7,10)

Adjustment Curve at nominal pH	Applied Voltage (mV)	Nominal Value (pH)	UUC Reading		Correction (mV)	Uncertainty (± mV)
			(pH)	(mV)		
4, 7, 10	177.4800	4	4.00	177.5	0.0	0.12
	0.0000	7	7.00	0.1	-0.1	0.086
	-177.4800	10	10.00	-177.4	-0.1	0.12

Function : pH meter with electrode

Performing a three - buffer standard curve using buffer nominal pH (4,7,10)

Adjustment Curve at nominal pH	Standard Buffer (pH)	UUC Reading (pH)	Correction (pH)	Uncertainty (± pH)
4, 7, 10	4.008	4.01	0.00	0.0097
	6.986	7.00	-0.01	0.011
	9.997	10.01	-0.01	0.014

Remark

UUC : Unit Under Calibration

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

- oOo -



CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhprachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech.cal@yahoo.com, calibratech.cal@hotmail.com



NSC-TISI-TIS 17025
CALIBRATION 0030

Certificate of Calibration

Certificate No. : 67-400454-3

Page : 1 of 2

Submitted by : Pacific Laboratory Co., Ltd

14/5358 Moo 14, T. Bang Bua Thong, A. Bang Bua Thong, Nonthaburi 11110 Thailand

Equipment : Temperature controlled enclosure (Incubator)

Manufacturer : Aqua Lytic

Model : TC 135S

Range : N/A °C

Resolution : 0.1 °C

Serial No. : 0614/000033

ID No. : LAB-IB-001

Environment : On site calibration was carried out at the Laboratory, Pacific Laboratory Co., Ltd

Ambient Temperature : (25.5 to 26.0) °C

Relative Humidity : (40 to 45) %

Line Voltage : (220.0 to 222.0) V

Date of Received : 30 July 2024

Date of Calibration : 30 July 2024

Date of Issue : 03 August 2024

Calibrated by : Permpon Chanpu

Calibration Method : CAL-M4004, TLAS G-20

The temperature scale used was based on ITS-90

Reference Standard Instruments : This certification is traceable to the International System of Units
Standard Digital Thermometer with RTD Probe

ID No.

Cert. No.

Due Date

Traceability

400029 & 400043 67-400245-1

27 Oct 2024

National Institute of Metrology Thailand (NIMT)

Approved by :

(Surachai Promthong)

Laboratory Manager

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 67-400454-3


Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Function : Temperature measurement

This instrument was setting air ventilation at position 0 (close)

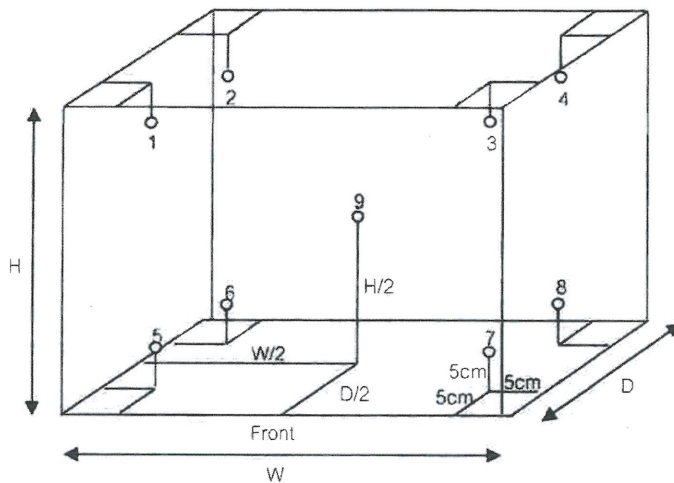

Inside of Chamber

W = 0.51 m

D = 0.04 m

H = 0.70 m

Capacity = 0.02 m³

Test Point (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Temperature (°C) @ Sensor No.									Uncertainty (± °C)
			1	2	3	4	5	6	7	8	9	
20.0	20.5	20.5	20.07	19.92	19.95	19.93	19.93	19.92	19.92	19.96	19.88	0.67

Test Point (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Uniformity (°C)	Measured Stability (°C)	Overall Variation (°C)
20.0	20.5	20.5	0.41	0.33	0.70

Remark The uncertainty is not combine uniformity of the air chamber

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

- o0o -



CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhprachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech.cal@yahoo.com, calibratech.cal@hotmail.com



NSC-TISI-TIS 17025
CALIBRATION 0030

Certificate of Calibration

Certificate No. : 67-400454-2

Page : 1 of 2

Submitted by : Pacific Laboratory Co., Ltd

14/5358 Moo 14, T. Bang Bua Thong, A. Bang Bua Thong, Nonthaburi 11110 Thailand

Equipment : Water Bath

Manufacturer : Memmert

Model : WNB 22

Range : N/A °C

Resolution : 0.1 °C

Serial No. : L514.0184

ID No. : LAB-WB-001

Environment : On site calibration was carried out at the Laboratory, Pacific Laboratory Co., Ltd

Ambient Temperature : (30.0 to 31.3) °C

Relative Humidity : (60 to 65) %

Line Voltage : (220.0 to 222.0) V

Date of Received : 30 July 2024

Date of Calibration : 30 July 2024

Date of Issue : 03 August 2024

Calibrated by : Permpon Chanpu

Calibration Method : This instrument was calibrated by In-house method CAL-M4006 based on ASTM E715-80
The temperature scale used was based on ITS-90

Reference Standard Instruments : This certification is traceable to the International System of Units
Standard Digital Thermometer with RTD probe

<u>ID No.</u>	<u>Cert. No.</u>	<u>Due Date</u>	<u>Traceability</u>
400029 & 400031	67-400244-1	24 Oct 2024	National Institute of Metrology Thailand (NIMT)

Approved by :

(Surachai Promthong)

Laboratory Manager

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration


Certificate No. : 67-400454-2

Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Function : Temperature measurement

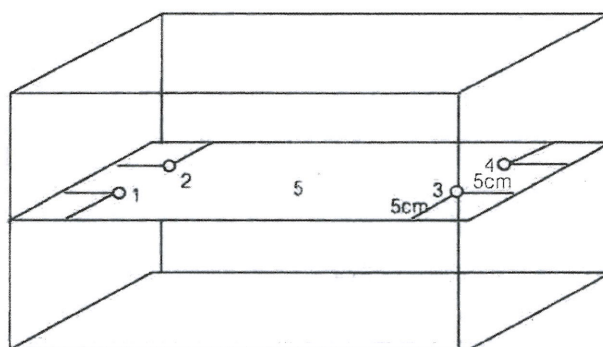

Front

Test Point (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Temperature (°C) @ Sensor					Uncertainty (± °C)	Measured Uniformity (°C)	Measured Stability (°C)
			No.							
			1	2	3	4	5			
65.0	65.0	65.0	64.61	64.70	64.66	64.64	64.68	0.18	0.12	0.05
95.0	95.0	95.0	94.60	94.69	94.70	94.61	94.70	0.18	0.15	0.03

Remark The uncertainty is not combine uniformity of the water bath

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

- o0o -

Handwritten signature



CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhprachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech.cal@yahoo.com, calibratech.cal@hotmail.com



NSC-TISI-TIS17025
CALIBRATION 0030

Certificate of Calibration

Certificate No. : 67-400454-1

Page : 1 of 2

Submitted by : Pacific Laboratory Co., Ltd

14/5358 Moo 14, T. Bang Bua Thong, A. Bang Bua Thong, Nonthaburi 11110 Thailand

Equipment : Temperature controlled enclosure (Oven)

Manufacturer : Memmert

Model : UN 55

Range : N/A °C

Resolution : 0.1 °C

Serial No. : B214.1879

ID No. : LAB-OV-001

Environment : On site calibration was carried out at the Laboratory, Pacific Laboratory Co., Ltd

Ambient Temperature : (30.0 to 31.3) °C

Relative Humidity : (60 to 65) %

Line Voltage : (220.0 to 222.0) V

Date of Received : 30 July 2024

Date of Calibration : 30 July 2024

Date of Issue : 03 August 2024

Calibrated by : Permpoon Chanpu

Calibration Method : CAL-M4004, TLAS G-20

The temperature scale used was based on ITS-90

Reference Standard Instruments : This certification is traceable to the International System of Units
Standard Digital Thermometer with Thermocouple probe

ID No.

Cert. No.

Due Date

Traceability

400029 & 400030

67-400246-1

25 Oct 2024

National Institute of Metrology Thailand (NIMT)

Approved by :

(Surachai Promthong)

Laboratory Manager

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.

CAL-F0031-03



Certificate of Calibration

Certificate No. : 67-400454-1


Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Function : Temperature measurement

This instrument was setting air ventilation at position 0 (close)

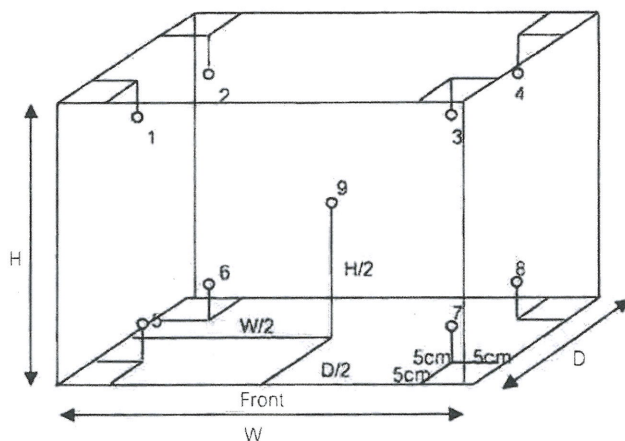

Inside of Chamber

W = 0.40 m

D = 0.33 m

H = 0.40 m

Capacity = 0.05 m³

Test Point (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Temperature (°C) @ Sensor No.									Uncertainty (± °C)
			1	2	3	4	5	6	7	8	9	
104.0	107.0	107.0	105.1	104.9	104.8	104.8	102.9	103.6	103.7	104.1	103.9	0.84
180.0	184.0	184.0	180.5	180.5	180.3	179.7	176.8	177.2	178.1	181.2	179.5	1.4

Test Point (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Uniformity (°C)	Measured Stability (°C)	Overall Variation (°C)
104.0	107.0	107.0	1.4	0.4	2.5
180.0	184.0	184.0	3.3	0.7	5.6

Remark The uncertainty is not combine uniformity of the air chamber

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k = 2 , providing a level of confidence of approximately 95%

- o0o -



Certificate of Calibration

Certificate No. : 67-400217-1

Page : 1 of 2

Submitted by : Special Lab Envi and Consultant Co., Ltd.
47/91 Moo 3 Thambol Tha-it, Pakkret, Nonthaburi 11120

Equipment : Temperature controlled enclosure(Incubator)
Manufacturer : Lovibond Model : FKU 1800
Range : N/A °C Resolution : 0.1 °C
Serial No. : 0925481-19 ID No. : LB-Eq-005

Environment : On site calibration was carried out at the Laboratory, Special Lab Envi and Consultant Co., Ltd.
Ambient Temperature : (24.0 to 25.0) °C
Relative Humidity : (50 to 55) %
Line Voltage : (226.0 to 226.5) V

Date of Received : 20 April 2024

Date of Calibration : 20 April 2024

Date of Issue : 26 April 2024

Calibrated by : Kittisak Kokaeo

Calibration Method : CAL-M4004, TLAS G-20

The temperature scale used was based on ITS-90

Reference Standard Instruments : This certification is traceable to the International System of Units
Standard Digital Thermometer with RTD Probe

ID No.	Cert. No.	Due Date	Traceability
400046 & 400047	67-400047-2	26 Jul 2024	National Institute of Metrology Thailand (NIMT)

Approved by :



(Surachai Promthong)

Laboratory Manager

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 67-400217-1


Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Function : Temperature measurement

This instrument was setting air ventilation at position 0 (close)

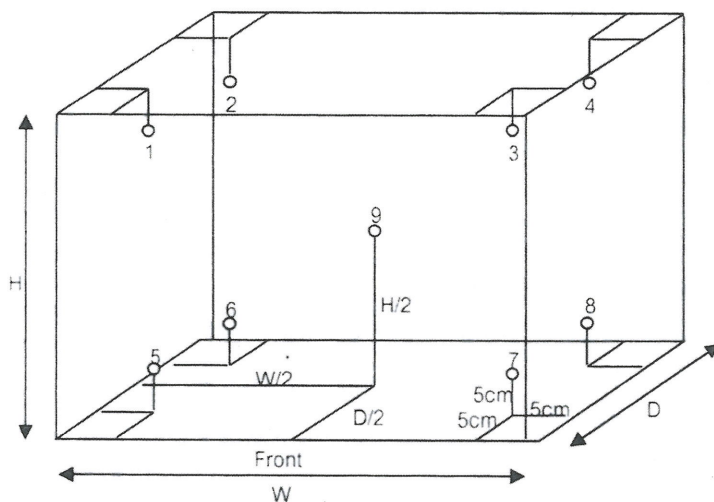

Inside of Chamber

W = 0.55 m

D = 0.73 m

H = 0.50 m

Capacity = 0.20 m³

Test Point (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Temperature (°C) @ Sensor No.									Uncertainty (± °C)
			1	2	3	4	5	6	7	8	9	
30.0	30.0	30.0	30.09	30.21	30.18	30.17	30.52	30.49	30.13	30.32	30.13	0.31
35.0	35.0	35.0	34.95	35.17	35.13	35.14	35.62	35.67	35.04	35.40	35.19	0.32
37.0	37.0	37.0	36.94	37.16	37.13	37.11	37.60	37.64	37.02	37.37	37.16	0.33

Test Point (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Uniformity (°C)	Measured Stability (°C)	Overall Variation (°C)
30.0	30.0	30.0	0.42	0.03	0.46
35.0	35.0	35.0	0.50	0.04	0.77
37.0	37.0	37.0	0.51	0.06	0.79

Remark The uncertainty is not combine uniformity of the air chamber

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

- o0o -

ABJ



Certificate of Calibration

Certificate No. : 67-300432-1

Page : 1 of 2

Submitted by : Special Lab Envi and Consultant Co., Ltd.

47/91-93 Moo 3, Tambol Tha-It, Pakkret, Nonthaburi 11120

Equipment : Piston Pipette

Manufacturer : sartorius

Model : N/A

Serial No. : 4541601431

ID No. : LB-Eq-045

Capacity : 100 μ l to 1000 μ l Resolution : 1 μ l

Environment : Ambient Temperature : (20 \pm 3) $^{\circ}$ C

Relative Humidity : (55 \pm 10) %

Air Pressure : (1008.1 to 1008.3) mbar.

Date of Received : 02 August 2024

Date of Calibration : 05 August 2024

Date of Issue : 05 August 2024

Calibrated by : Wipa Tovadee

Calibration Method : In-house method CAL-M3002 base on ISO 8655-6 : 2022-04

Reference Standard Instruments : This certification is traceable to the International System of Units

Electronic Balance

ID No.	Cert. No.	Due Date	Traceability
241003	67-200210-2	02 Dec 2024	National Institute of Metrology (Thailand) (NIMT)

Approved by :

(Wipa Tovadee)

Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 67-300432-1

Page : 2 of 2

Result of Calibration : Without Adjustment

based on the gravimetric determination of the quantity of water which is converted to true volume at the standard temperature of 20 °C

Setting Volume (μl)	Measuring Volume (μl)	e_s (μl)	η_s (%)	S_r (μl)	C_v (%)	Uncertainty ($\pm \mu\text{l}$)	Coverage Factor (k)
100	100.02	0.02	0.02	0.07	0.07	1.3	2.00
500	500.85	0.85	0.17	0.17	0.03	1.3	2.00
1000	1000.03	0.03	0.00	0.13	0.01	1.7	2.00

Note : e_s : Systematic error (μl) , η_s : Relative systematic error (%)

S_r : Standard deviation (μl) , C_v : Coefficient of variation (%)

The formula used to convert weighing values into volume is

$$V_{20} = M \times Z$$

V_{20} = is the water volume at standard temperature of 20 °C

M = is the balance reading of delivered water

Z = is the combined factor for buoyancy correction and conversion from mass to volume

UUC Condition As-Received : Good

UUC Calibrated to delivery (Ex) by using : White Tip

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor (k)

providing a level of confidence of approximately 95%

- o0o -

