

เอกสารรับรองการสอบเทียบ ของเครื่องมือวัด





บริษัท เอ็นไวแล็บ จำกัด 540,540/1 ซอยบางแค 7 แขวงบางแค เขตบางแค กรุงเทพฯ 10160
Envilab Co., Ltd. 540,540/1 Soi Bangkhoe 7 Bangkhoe Bangkok Bangkok 10160
Tel : 02-802-3577-8 Fax: 02-802-3773 E-mail : info@evltesting.com



Envilab & Network Supply Instrument

TSP High Volume Sampler Calibration

Verification Report No.

SO2200267-E001 -TSP 01

<input type="checkbox"/> PM	<input checked="" type="checkbox"/> Onsite
Site: บริเวณใกล้กับท่าเรือ	
UTM : 47P N 1505157 E 668815	
Sampler: ETSP#38	
Recorder: ECRAN000031073	
Date: 11 Oct 24	
Technical: Amonthep Konklee	
Approval: Wisan Ritthikamon	

CONDITIONS

Barometric Press. (hPa): 989.0	Corrected Pressure (mm Hg): 741.8
Temperature (deg C): 38.0	Temperature (deg K): 311.0
Average Press. (hPa): 1013.0	Corrected Avg. Press. (mm Hg): 759.8
Average Temp. (deg C): 30.0	Average Temp. (deg K): 303.0


CALIBRATION ORIFICE

Brand: Tisch Environmental, Inc
Model: TC-5025A
Serial#: 5411

Qstd Slope: 2.02024
Qstd Intercept: -0.02667
Date Certified: 9 Feb 2024
Due Date : 08-Feb-25

CALIBRATIONS

Plate or Test #	H2O (in)	Qstd (m3/min)	I (chart)	IC (corrected)	LINEAR REGRESSION
1	12.20	1.685	58.0	56.09	
2	9.60	1.496	52.0	50.29	Slope = 29.8465 Intercept = 5.0821 Corr. coeff.= 0.9942 # of Observations: 5 Range of Chart at 1.1 - 1.7 m3/min.: 40 57
3	7.50	1.324	44.0	42.55	
4	4.70	1.051	38.0	36.75	
5	2.60	0.785	30.0	29.01	

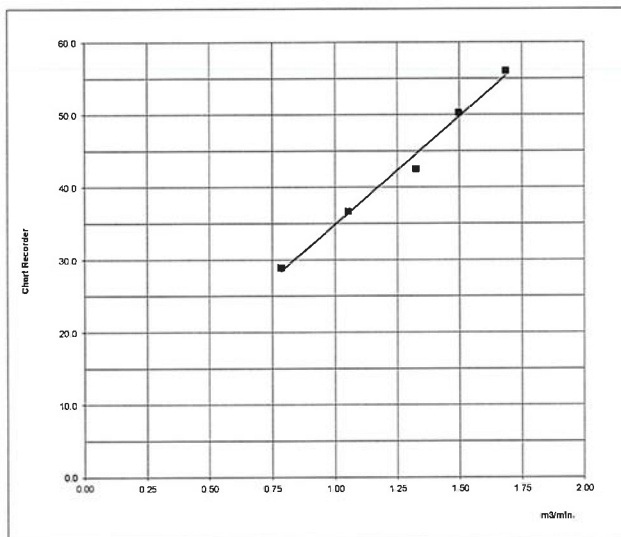

Calibrated by :

Amonthep Konklee
11 October 2024

Approved by :

Wisan Ritthikamon
11 October 2024

This report shall not be reproduced except in full, without the written approval of Envilab Co., Ltd.

www.evltesting.com

Environmental responsibility with accuracy measurement

FE MNT-29 Rev. 02/05/07/67



รับรองสำเนาถูกต้อง
ผู้จัดการฝ่ายควบคุมคุณภาพ



บริษัท เอ็นไวแล็บ จำกัด 540,540/1 ซอยบางแค 7 แขวงบางแค เขตบางแค กรุงเทพฯ 10160
Envilab Co., Ltd. 540,540/1 Soi Bangkhae 7 Bangkhae Bangkok Bangkok 10160
Tel : 02-802-3577-8 Fax. 02-802-3773 E-mail : info@evltesting.com



Envilab: R. Nongkhae Supply Instrument

TSP High Volume Sampler Calibration

Verification Report No.

SO2200267-E001 -TSP 02

☐ PM ☒ Onsite

Site: บริเวณท่าเทียบเรือ

UTM : 47P N 1505248 E 668810

Sampler: ETSP#39

Recorder: ECRAN000031074

Date: 11 Oct 24

Technical: Amonthep Konklee

Approval: Wisan Ritthikamon

CONDITIONS

Barometric Press. (hPa): 989.0

Temperature (deg C): 38.0

Average Press. (hPa): 1013.0

Average Temp. (deg C): 30.0

Corrected Pressure (mm Hg): 741.8

Temperature (deg K): 311.0

Corrected Avg. Press. (mm Hg): 759.8

Average Temp. (deg K): 303.0

CALIBRATION ORIFICE

Brand: Tisch Environmental, Inc

Model: TE-5025A

Serial#: 5411

Qstd Slope: 2.02024

Qstd Intercept: -0.02667

Date Certified: 9 Feb 2024

Due Date : 08-Feb-25

CALIBRATIONS

Plate or Test #	H2O (in)	Qstd (m3/min)	I (chart)	IC (corrected)
1	12.20	1.685	56.0	54.16
2	8.60	1.417	50.0	48.35
3	6.40	1.224	42.0	40.62
4	4.00	0.971	36.0	34.82
5	2.20	0.723	30.0	29.01

LINEAR REGRESSION


Slope = 26.8160

Intercept = 9.1033

Corr. coeff. = 0.9955

of Observations: 5

Range of Chart at 1.1 - 1.7 m3/min. 40 56

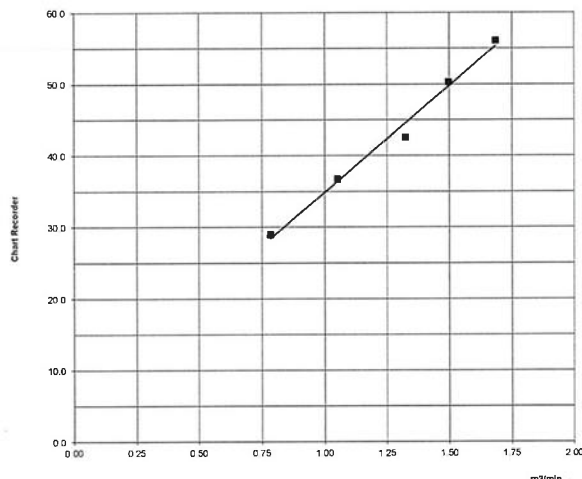

Calibrated by :

Amonthep Konklee
11 October 2024

Approved by :

Wisan Ritthikamon
11 October 2024

This report shall not be reproduced except in full, without the written approval of Envilab Co., Ltd.

www.evltesting.com

Environmental responsibility with accuracy measurement

FE-MNT-29 Rev.02:05/07/67



รับรองสำเนาถูกต้อง
ผู้จัดการฝ่ายควบคุมคุณภาพ



บริษัท เอ็นไวแล็บ จำกัด 540.540/1 ซอยบางแค 7 แขวงบางแค เขตบางแค กรุงเทพฯ 10160
Envilab Co., Ltd. 540.540/1 Soi Bangkhoe 7 Bangkhoe Bangkok Bangkok 10160
Tel : 02-802-3577-8 Fax: 02-802-3773 E-mail : info@evltesting.com



Envilab is Needles Supply Instrument

PM10 High Volume Sampler Calibration

Verification Report No.

SO2200267-E001 -PM 01

☐ PM ☒ Onsite

Site: บริเวณโถงใต้เก็บทรายแก้ว

UTM : 47P N 1505157 E 668815

Sampler: EPM10#29

Recorder: ECRDS016431075

Date: 11 Oct 24

Technical: Amonthep Konklee

Approval: Wisan Ritthikamon

CONDITIONS

Barometric Press. (hPa): 989.0

Temperature (deg C): 38.0

Average Press. (hPa): 1013.0

Average Temp. (deg C): 30.0

Corrected Pressure (mm Hg): 741.8

Temperature (deg K): 311.0

Corrected Avg. Press. (mm Hg): 759.8

Average Temp. (deg K): 303.0

CALIBRATION ORIFICE

Brand: Tisch Environmental, Inc

Model: TE-5025A

Serial#: 5411

Qstd Slope: 1.2654

Qstd Intercept: -0.01667

Date Certified: 9 Feb 2024

Due Date : 08-Feb-25

CALIBRATIONS

Plate or Test #	H2O (in)	Qa (m3/min)	I (chart)	IC (corrected)
1	12.20	1.800	48.0	31.08
2	9.50	1.590	43.0	27.84
3	7.30	1.396	36.0	23.31
4	4.70	1.122	30.0	19.42
5	2.70	0.854	22.0	14.24

LINEAR REGRESSION

Slope = 17.7895

Intercept = -0.8814

Corr. coeff. = 0.9980


SFR = 1.188

SSP = 31.28

of Observations: 5

Range of Chart 29

at SFR $\pm 10\%$ 34

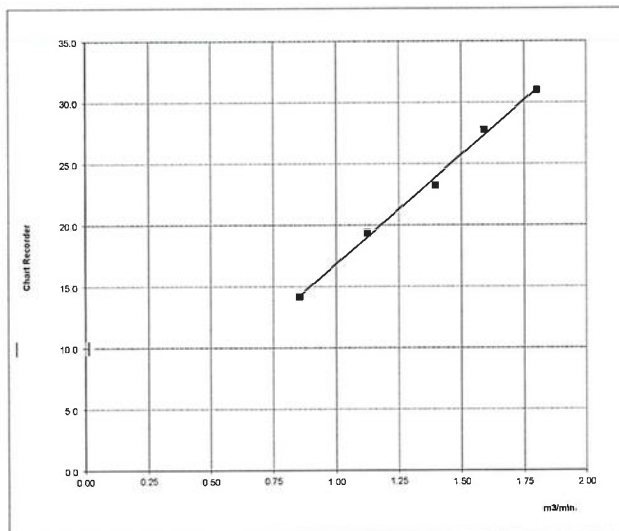

Calibrated by :

Amonthep Konklee
11 October 2024

Approved by :

Wisan Ritthikamon
11 October 2024

This report shall not be reproduced except in full, without the written approval of Envilab Co., Ltd.

www.evltesting.com

Environmental responsibility with accuracy measurement

FE-MINT-29 Rev 02:05/07/67



รับรองสำเนาถูกต้อง
ผู้จัดการฝ่ายควบคุมคุณภาพ



บริษัท เอ็นไวเลบ จำกัด 540,540/1 ซอยบางแค 7 แขวงบางแค เขตบางแค กรุงเทพฯ 10160
Envilab Co., Ltd. 540,540/1 Soi Bangkhoe 7 Bangkhoe Bangkok Bangkok 10160
Tel : 02-802-3577-8 Fax. 02-802-3773 E-mail : info@evltesting.com



Envilab & Needles Supply Instrument

PM10 High Volume Sampler Calibration

Verification Report No.

SO2200267-E001 -PM 02

<input type="checkbox"/> PM	<input checked="" type="checkbox"/> Onsite
Site: <u>บริเวณท่าเทียบเรือ</u>	
UTM: <u>47P N 1505248 E 668810</u>	
Sampler: <u>EPM10#32</u>	
Recorder: <u>ECRDS016449814</u>	
Date: <u>11 Oct 24</u>	
Technical: <u>Amonthep Konklee</u>	
Approval: <u>Wisani Ritthikamon</u>	

CONDITIONS

Barometric Press. (hPa): 989.0	Corrected Pressure (mm Hg): 741.8
Temperature (deg C): 38.0	Temperature (deg K): 311.0
Average Press. (hPa): 1013.0	Corrected Avg. Press. (mm Hg): 759.8
Average Temp. (deg C): 30.0	Average Temp. (deg K): 303.0


CALIBRATION ORIFICE

Brand: Tisch Environmental, Inc
Model: TE-5025A
Serial#: 5411


Qstd Slope: 1.2654
Qstd Intercept: -0.01667
Date Certified: 9 Feb 2024
Due Date: 08-Feb-25

CALIBRATIONS

Plate or Test #	H2O (in)	Qa (m3/min)	I (chart)	IC (corrected)	LINEAR REGRESSION
1	11.40	1.741	50.0	32.37	Slope = 17.7561
2	8.80	1.531	44.0	28.49	Intercept = 1.0296
3	6.60	1.328	36.0	23.31	Corr. coeff. = 0.9935
4	3.90	1.024	30.0	19.42	SFR = 1.188
5	2.80	0.869	26.0	16.83	SSP = 34.17
					# of Observations: 5
					Range of Chart at SFR $\pm 10\%$
					32
					36

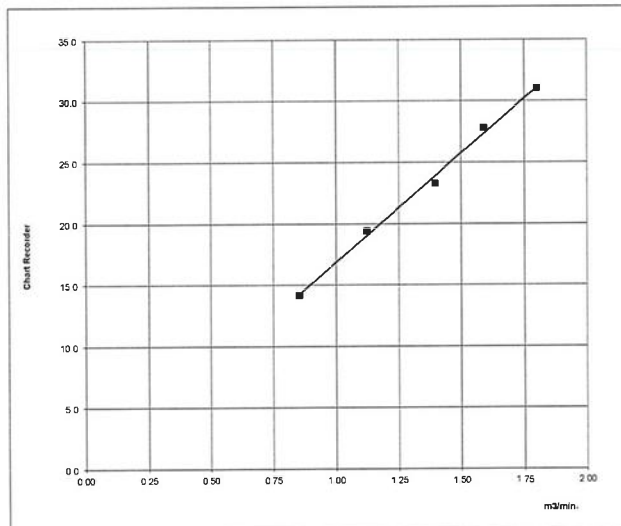

Calibrated by : 
Amonthep Konklee
11 October 2024

Approved by : 
Wisani Ritthikamon
11 October 2024

This report shall not be reproduced except in full, without the written approval of Envilab Co., Ltd.

www.evltesting.com

Environmental responsibility with accuracy measurement

PM10 Cal. Rev 07 / Iss Date Mar 17, 2020

FE-MNT-29 Rev 02/05/07/67



รับรองสำเนาถูกต้อง
ผู้จัดการฝ่ายควบคุมคุณภาพ



Certificate of Calibration

Calibration Certification Information

Cal. Date: February 9, 2024 Rootsmeter S/N: 438320 Ta: 295 °K
 Operator: Jim Tisch Pa: 749.0 mm Hg
 Calibration Model #: TE-5025A Calibrator S/N: 5411

Run	Vol. Init (m3)	Vol. Final (m3)	ΔVol. (m3)	ΔTime (min)	ΔP (mm Hg)	ΔH (in H2O)
1	1	2	1	1.3950	3.2	2.00
2	3	4	1	0.9840	6.4	4.00
3	5	6	1	0.8790	7.9	5.00
4	7	8	1	0.8430	8.8	5.50
5	9	10	1	0.6940	12.7	8.00

Data Tabulation

Vstd (m3)	Qstd (x-axis)	$\sqrt{\Delta H \left(\frac{Pa}{Pstd} \right) \left(\frac{Tstd}{Ta} \right)}$ (y-axis)	Va	Qa (x-axis)	$\sqrt{\Delta H \left(\frac{Ta}{Pa} \right)}$ (y-axis)
0.9914	0.7106	1.4111	0.9957	0.7138	0.8875
0.9871	1.0032	1.9956	0.9915	1.0076	1.2551
0.9851	1.1207	2.2312	0.9895	1.1257	1.4033
0.9839	1.1672	2.3401	0.9883	1.1723	1.4718
0.9787	1.4103	2.8222	0.9830	1.4165	1.7750
QSTD	m=	2.02024	QA	m=	1.26504
	b=	-0.02667		b=	-0.01677
	r=	0.99993		r=	0.99993

Calculations

Vstd=	$\Delta Vol \left(\frac{Pa - \Delta P}{Pstd} \right) \left(\frac{Tstd}{Ta} \right)$	Va=	$\Delta Vol \left(\frac{Pa - \Delta P}{Pa} \right)$
Qstd=	Vstd/ΔTime	Qa=	Va/ΔTime
For subsequent flow rate calculations:			
Qstd=	$1/m \left(\left(\sqrt{\Delta H \left(\frac{Pa}{Pstd} \right) \left(\frac{Tstd}{Ta} \right)} \right) - b \right)$	Qa=	$1/m \left(\left(\sqrt{\Delta H \left(\frac{Ta}{Pa} \right)} \right) - b \right)$

Standard Conditions

Tstd:	298.15 °K
Pstd:	760 mm Hg
Key	
ΔH: calibrator manometer reading (in H2O)	
ΔP: rootsmeter manometer reading (mm Hg)	
Ta: actual absolute temperature (°K)	
Pa: actual barometric pressure (mm Hg)	
b: intercept	
m: slope	

RECALIBRATION

US EPA recommends annual recalibration per 1998 40 Code of Federal Regulations Part 50 to 51, Appendix B to Part 50, Reference Method for the Determination of Suspended Particulate Matter in the Atmosphere, 9.2.17, page 30



Certificate of Calibration

Certificate No. : 67-200060-1

Page : 1 of 2

Submitted by : Envilab Co., Ltd.
540, 540/1 Soi Bangkhao7, Bangkhao, Bangkok 10160

Equipment : Electronic Balance
Manufacturer : Sartorius **Model :** SECURA125-1S
Serial No. : 0034606552 **ID No. :** ELABBALANCEN05
Capacity : 120 g **Resolution :** 0.0001 g

Environment : On site calibration was carried out at the B304 Balance Room, Envilab Co., Ltd.
Ambient Temperature : (20.0 to 20.7) °C
Relative Humidity : (56.2 to 60.3) %
Air Pressure : 1013.0 mbar

Date of Received : 20 February 2024

Date of Calibration : 20 February 2024

Date of Issue : 21 February 2024

Calibrated by : Satja Sangkhum

Calibration Method : In-house method CAL-M2001 based on UKAS Publication ref : LAB 14
Edition 7 - November 2022

Reference Standard Instruments : This certification is traceable to the International System of Units

Standard Weights

ID No.	Cert. No.	Due Date	Traceability
E261-E2624	C02232088	08 Nov 2024	National Institute of Metrology (Thailand), (NIMT)

Approved by :

(Surachai Promthong)

Laboratory Manager

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Envilab Co.,Ltd.

รับรองสำเนาถูกต้อง

ผู้จัดการฝ่ายควบคุมคุณภาพ



Certificate of Calibration

Certificate No. : 67-410025-1

Page : 1 of 2

Submitted by : Envilab Co., Ltd.
540, 540/1 Soi Bangkhac 7, Bangkhac, Bangkok 10160

Equipment : Digital Thermo-Hygrometer

Manufacturer : Jedto

Model : HTC-1

Range Temperature : N/A °C

Resolution : 0.1 °C

Range Humidity : N/A %R.H.

Resolution : 1 %R.H.

Serial No. : PONPE5852094

ID No. : ELABTMHTC10003

Environment : Ambient Temperature : $(23 \pm 2) ^\circ\text{C}$
Relative Humidity : $(50 \pm 15) \%$

Date of Received : 20 February 2024

Date of Calibration : 22 February 2024

Date of Issue : 22 February 2024

Calibrated by : Chortip Samchusri

Calibration Method : This instrument was calibrated by In-house method comparison technique CAL-M4013 by compared with standard probe sensor humidity/temperature into humidity/temperature chamber.

Reference Standard Instruments : This certification is traceable to the International System of Units
Digital Indicator with Standard Probe Temp&Hum

ID No.	Cert. No.	Due Date	Traceability
400034 & 400035	SG-H-00020/67	05 Jul 2024	Success Gateway Co., Ltd., Accredited by TISI Calibration No.0268

Approved by :



(Surachai Promthong)

Laboratory Manager



รับรองสำเนาถูกต้อง

Envilab Co.,Ltd. ผู้จัดการฝ่ายควบคุมคุณภาพ



The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.

CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhprachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech.cal@yahoo.com, calibratech.cal@hotmail.com

Certificate of Calibration

Certificate No. : 67-410025-1

Page : 2 of 2

UUC Condition As-Received : Good

Result of Calibration : Without Adjustment

Function : Temperature measurement

Reference Humidity @ 50 %R.H.

Standard Temperature (°C)	UUC Reading (°C)	Correction (°C)	Uncertainty (± °C)
24.98	25.0	0.0	0.46

Result of Calibration : Without Adjustment

Function : Humidity measurement

Reference Temperature @ 25 °C

Standard Humidity (%R.H.)	UUC Reading (%R.H.)	Correction (%R.H.)	Uncertainty (± %R.H.)
50.03	50	0	2.2

Remark

UUC : Unit Under Calibration

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

- o0o -



Envilab Co.,Ltd.

รับรองสำเนาถูกต้อง
ผู้จัดการฝ่ายควบคุมคุณภาพ





THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804,0-2399-0469

Calibration Certificate

Issued by : Calibration & Test Section : Meteorological Instruments Bureau

Date of Issue 6 April, 2024

Certification No. 172/24

Page : 1 of 6

Object : เครื่องมือตรวจวัดอุตุนิยมวิทยา

Manufacturer : NovaLynx

Type : Data Logger 110-WS-25DL-D

Serial No. : EWSNV110WS2503

Customer : ENVILAB Co.,Ltd.
540, 540/1 Soi Bangkhae 7, Bangkhae, Bangkhae,
Bangkok 10160,Thailand.

Calibration Condition : Temperature 25.1 °C Barometric Pressure 1009.2 hPa

NATIONAL STANDARD WIND TUNNEL : Wind Aloft Plotting Board

: Micromanometer Theodor Friedrichs FC014 Serial No. 9310119 : HOOK GAGE NO 1425

N.I.S.T. Test Reference Number 731/241460 : Standard Velocity at 20 - 30 m/sec


: Ultrasonic Anemometer Model DA-650-3TV (sensor TR-90AH)
Serial Number 110730029 (sensor 120629586)

JAPAN QUALITY ASSURANCE ORGANIZATION : Standard Velocity at 0 - 20 m/sec


STANDARD THERMOMETER : Theodor Friedrich : Dry No.8390/94 Wet No. 8389/94

: Thermoschneider No.9188 : testo, testo 645 Serial No. 02848057

STANDARD BAROMETER : Digital Barometer Vaisala Type PTB220 No. V1220015

Calibrated by : 

Mr. Watcharapol Subwat
Mechanical Engineer

Signed : 
Mr. Pisood Promsut

(Authorised Signatory)
for the Chief
Sub-Standard Instrument



รับรองสำเนาถูกต้อง
ผู้จัดการฝ่ายควบคุมคุณภาพ
Envilab Co.,Ltd.



THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804,0-2399-0469

The Result of Calibration

Sensor model

EWSNV110WS2503

Certification No. 172/24

6 April, 2024

Page : 2 of 6

Standard Ultrasonic Anemometer m/sec	HOOK GAGE NO. 1425			TESTED ANEMOMETER	
	Pressure	Vacumm	Velocity	Velocity	Correction
	inches H2O	inches H2O	m/sec	m/sec	m/sec
1.00	-	-	-	0.3	0.70
3.02	-	-	-	2.4	0.62
5.00	-	-	-	4.9	0.10
7.04	-	-	-	6.9	0.14
9.02	-	-	-	8.8	0.22
11.01	-	-	-	10.9	0.11
13.01	-	-	-	12.8	0.21
15.01	-	-	-	15.1	-0.09
17.02	-	-	-	16.8	0.22
20.02	-	-	-	20.1	-0.08

Wind Aloft Plotting Board.	
US.DEPARTMENT OF COMMERCE WEATHER BUREAU	
WIND DIRETION	TESTED WIND DIRECTION
0	0
90	91
180	179
270	270

Calibrated by :

Watchapol

Mr. Watchapol Subwat

Mechanical Engineer

Calibration & Test Section

Meteorological Instruments Bureau



Envilab Co.,Ltd.

รับรองสำเนาถูกต้อง

ผู้จัดการฝ่ายควบคุมคุณภาพ



THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804, 0-2399-0469

The Result of Calibration

Sensor model

EWSNV110WS2503

Certification No. 172/24

6 April, 2024

Page : 3 of 6

Standard Barometer	Tested Barometer	Correction
Pressure	Pressure	
1009.59	1010.02	-0.43
1009.45	1009.95	-0.50
1010.10	1010.53	-0.43
1010.94	1011.36	-0.42
1011.46	1011.85	-0.39
1011.84	1012.34	-0.50
1012.06	1012.47	-0.41
1013.04	1013.48	-0.44
1013.18	1013.56	-0.38
1012.89	1013.27	-0.38
1013.20	1013.61	-0.41
1013.44	1013.85	-0.41
1013.81	1014.21	-0.40
1014.19	1014.68	-0.49
1015.96	1016.32	-0.36
1016.23	1016.65	-0.42
1015.64	1016.03	-0.39
1015.23	1015.68	-0.45
1012.87	1013.31	-0.44
1013.63	1014.10	-0.47

Average

Calibrated by :

Watcharapol

Mr. Watcharapol Subwat

Mechanical Engineer

Calibration & Test Section
Meteorological Instruments Bureau



รับรองสำเนาถูกต้อง
ผู้จัดการฝ่ายควบคุมคุณภาพ



THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804, 0-2399-0469

The Result of Calibration

Sensor model

EWSNV110WS2503

Certification No. 172/24

6 April, 2024

Page : 4 of 6

Standard Temp. °C	Temperature Sensor Reading	
	Reading °C	Correction °C
45.6	46.0	-0.4
30.1	30.3	-0.2
15.4	15.7	-0.3

Calibrated by :

Watcharapol

Mr. Watcharapol Subwat

Mechanical Engineer

Calibration & Test Section
Meteorological Instruments Bureau



Envilab Co., Ltd.

รับรองสำเนาถูกต้อง
ผู้จัดการฝ่ายควบคุมคุณภาพ



THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804,0-2399-0469

The Result of Calibration

Sensor model EWSNV110WS2503 Certification No. 172/24

6 April, 2024

Page : 5 of 6

Standard Humidity % R.H.	Relative Humidity Sensor Reading	
	Reading	Correction
	% R.H.	% R.H.
85.2	91.5	-6.3
62.4	67.7	-5.3
41.5	46.2	-4.7

Calibrated by :

Watcharapol

Mr. Watcharapol Subwat
Mechanical Engineer



Envilab Co.,Ltd.

รับรองสำเนาถูกต้อง
ผู้จัดการฝ่ายควบคุมคุณภาพ



Date of Issue 6 April, 2024

Certification No. 172/24

Page: 6 of 6

ใบรับรอง

หนังสือฉบับนี้ขอรับรองว่า เครื่องวัดฝน ยี่ห้อ Davis Instruments แบบ TIPPING
BUCKET Product No. #7852 Mfg. Code. EWSNV110WS2503 ทำการสอบเทียบกับแก้ววัดฝน
แบบแก้วดวง GAUGE DIAMETER 8.0 INCHES, NEGRETTI & ZAMBRA LONDON No.
71082 และสามารถนำไปใช้ได้ มีค่าถูกต้องตามรายละเอียดของเครื่องมือ (0.2 mm./TIP)



ลงชื่อ.....

(นายวัชรพล ทรัพย์วัฒน์)

วิศวกรชำนาญการ



รับรองสำเนาถูกต้อง
ผู้จัดการฝ่ายควบคุมคุณภาพ



THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804, 0-2399-0469

Calibration Certificate

Issued by : Calibration & Test Section : Meteorological Instruments Bureau

Date of Issue 6 April, 2024

Certification No. 170/24

Page : 1 of 6

Object : เครื่องมือตรวจวัดอุณหภูมิ

Manufacturer : DYACON

Type : Data Logger MS-100

Serial No. : 130150 ID No. : EWSDCMS1200150

Customer : ENVILAB Co.,Ltd.
540,540/1 Soi Bangkhae 7, Bangkhae, Bangkhae,
Bangkok 10160, Thailand.

Calibration Condition : Temperature 25.1 °C Barometric Pressure 1008.7 hPa

NATIONAL STANDARD WIND TUNNEL : Wind Aloft Plotting Board

: Micromanometer Theodor Friedrichs FC014 Serial No. 9310119 : HOOK GAGE NO 1425

N.I.S.T. Test Reference Number 731/241460 : Standard Velocity at 20 - 30 m/sec

: Ultrasonic Anemometer Model DA-650-3TV (sensor TR-90AH)


Serial Number 110730029 (sensor 120629586)

JAPAN QUALITY ASSURANCE ORGANIZATION : Standard Velocity at 0 - 20 m/sec

STANDARD THERMOMETER : Theodor Friedrich : Dry No.8390/94 Wet No. 8389/94

: Thermoschneider No.9188 : testo, testo 645 Serial No. 02848057

STANDARD BAROMETER : Digital Barometer Vaisala Type PTB220 No. V1220015

Calibrated by : 

Mr. Watcharapol Subwat

Mechanical Engineer

Signed : 

Mr. Pisood Promsut

(Authorised Signatory)

for the Chief

Sub-Standard Instrument

Envilab Co.,Ltd.

รับรองสำเนาถูกต้อง
ผู้จัดการฝ่ายควบคุมคุณภาพ



THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804, 0-2399-0469

The Result of Calibration

Sensor Wind Speed & Wind Direction Model WSD-1 F Certification No. 170/24

6 April, 2024

Serial No. 1224

Page : 2 of 6

Standard	HOOK GAGE NO. 1425			TESTED ANEMOMETER	
Ultrasonic Anemometer	Pressure	Vacuum	Velocity	Velocity	Correction
m/sec	inches H ₂ O	inches H ₂ O	m/sec	m/sec	m/sec
1.00	-	-	-	1.0	0.00
3.02	-	-	-	2.9	0.12
5.00	-	-	-	5.0	0.00
7.04	-	-	-	7.0	0.04
9.02	-	-	-	9.0	0.02
11.01	-	-	-	11.0	0.01
13.01	-	-	-	12.9	0.11
15.01	-	-	-	15.0	0.01
17.02	-	-	-	17.0	0.02
20.02	-	-	-	20.0	0.02


Wind Aloft Plotting Board.	
US.DEPARTMENT OF COMMERCE WEATHER BUREAU	
WIND DIRECTION	TESTED WIND DIRECTION
0	0
90	91
180	180
270	

Calibrated by :

Watchapol

Mr. Watchapol Subwat

Mechanical Engineer

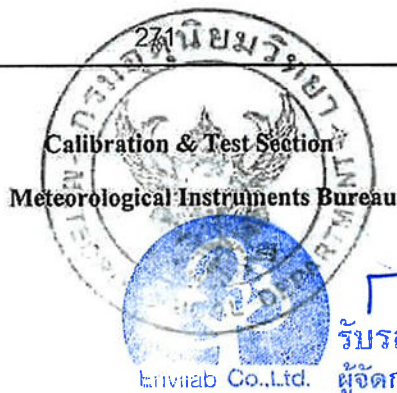

รับรองสำเนาถูกต้อง
ผู้จัดการฝ่ายควบคุมคุณภาพ



THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804, 0-2399-0469

The Result of Calibration

Sensor Pressure Model TPH-1 C

Serial No. 6275

Certification No. 170/24

6 April, 2024

Page : 3 of 6

Standard Barometer	Tested Barometer	Correction
Pressure	Pressure	
1009.59	1009.1	0.49
1009.45	1009.0	0.45
1010.10	1009.6	0.50
1010.94	1010.5	0.44
1011.46	1011.0	0.46
1011.84	1011.5	0.34
1012.06	1011.6	0.46
1013.04	1012.6	0.44
1013.18	1012.7	0.48
1012.89	1012.4	0.49
1013.20	1012.8	0.40
1013.44	1013.0	0.44
1013.81	1013.4	0.41
1014.19	1013.6	0.59
1015.96	1015.5	0.46
1016.23	1015.7	0.53
1015.64	1015.2	0.44
1015.23	1014.7	0.53
1012.87	1012.3	0.57
1013.63	1013.1	0.53

Average

0.47

Calibrated by :

Watchapol

Mr. Watchapol Subwat

Mechanical Engineer





THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804, 0-2399-0469

The Result of Calibration

Sensor Temperature Model TPH-1 C

Certification No. 170/24

6 April, 2024

Serial No. 6275

Page : 4 of 6

Standard Temp. °C	Temperature Sensor Reading	
	Reading °C	Correction °C
45.6	45.6	0.0
30.1	30.1	0.0
15.4	15.5	-0.1

Calibrated by :

Watchapol

Mr. Watchapol Subwat

Mechanical Engineer



Envilab Co., Ltd.

รับรองสำเนาถูกต้อง
ผู้จัดการฝ่ายควบคุมคุณภาพ



THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804, 0-2399-0469

The Result of Calibration

Sensor Humidity Model TPH-1 C

Certification No. 170/24

6 April, 2024

Serial No. 6275

Page : 5 of 6

Standard Humidity % R.H.	Relative Humidity Sensor Reading	
	Reading	Correction
	% R.H.	% R.H.
85.2	82.5	2.7
62.4	60.2	2.2
41.5	40.1	1.4

Calibrated by :

Watcharapol

Mr. Watcharapol Subwat

Mechanical Engineer

Calibration & Test Section
Meteorological Instruments Bureau



รับรองสำเนาถูกต้อง
ผู้จัดการฝ่ายควบคุมคุณภาพ



Date of Issue 6 April, 2024

Certification No. 170/24

Page: 6 of 6

ใบรับรอง

หนังสือฉบับนี้ขอรับรองว่า เครื่องวัดฝน ยี่ห้อ Davis Instruments แบบ TIPPING
BUCKET Product No. #7852 Mfg. Code. EWSDCMS1200150 ทำการสอบเทียบกับแก้ววัดฝน
แบบแก้วดวง GAUGE DIAMETER 8.0 INCHES, NEGRETTI & ZAMBRA LONDON No.
71082 และสามารถนำไปใช้ได้ มีค่าถูกต้องตามรายละเอียดของเครื่องมือ (0.2 mm./TIP)



ลงชื่อ..... รังสรรค์ กว-วิวัฒน์

(นายวัชรพล ทรัพย์วัฒน์)

วิศวกรชำนาญการ



Envilab Co., Ltd.

รับรองสำเนาถูกต้อง
ผู้จัดการฝ่ายควบคุมคุณภาพ



MIRACLE INTERNATIONAL TECHNOLOGY CO.,LTD

214 Bangwaek Rd. Bangpai Bangae Bangkok 10160
Tel.: 0-2865-4647-8 Fax: 0-2865-4649 <http://www.mit.in.th>



CALIBRATION CERTIFICATE

Certificate No. : L202408339-0001

Date Issued : 29-Aug-24

Customer : Envilab Co., Ltd.
540, 540/1 Soi Bangkhae 7, Bangkhae, Bangkok, Thailand 10160

Equipment : pH Meter

Manufacturer : ADWA

Model : AD12

Serial No. : 11105230175

ID No./Tag No. : ELABPHADWA1204

Date Received : 26-Aug-24

Date Calibrated : 27-Aug-24

Calibrated by : Sunisa Pinklao

Calibration Method or Calibration Procedure Used

In-house method : CP-42 by direct measurement with pH buffer solution.

This certificate is traceable to national standards, which realize the units of measurement according to the International System of Units (SI).

Result of Calibration

The reported uncertainty of measurement was based on standard uncertainty multiplied by a coverage factor $k = 2$, providing a level confidence approximately 95 percent.

This certificate may not be reproduced other than in full except with the prior written approval of the Miracle International Technology Company Limited.

Approved by:

Sorayuth T.
(Sarayuth Tochua)



Page 1 of 2



รับรองสำเนาถูกต้อง
ผู้จัดการฝ่ายควบคุมคุณภาพ

Certificate No : L202408339-0001

Environment : Ambient Temperature : $(25 \pm 2)^{\circ}\text{C}$
Relative Humidity : $(50 \pm 15)\%\text{RH}$

Electrode Test Results Part

2 points calibration using standard buffer solutions of pH 4.01, pH 7.01

Set Slope : - NIMT Lot No. 040822_2 for pH 4.003 Buffer Solution, Due 20 NOV 2024
- CPA chem Lot No. 1008799 for pH 7.0 Buffer Solution, Due 10 JUL 2026

Standard	Before Adjusted	After Adjusted	UUC Error	Uncertainty	MPE	Pass / Fail
pH Solution @ 25° C (pH)	UUC Reading (pH)	UUC Reading (pH)	(pH)	(\pm pH)	(\pm pH)	with Guard Band
4.003	4.20	4.00	-0.003	0.0091	0.1	Pass
6.984	7.18	6.98	-0.004	0.0084	0.1	Pass
10.003	9.78	9.92	-0.083	0.0085	0.1	Pass

STD = Standard

Pass = $|\text{error}| + |\text{uncertainty}| \leq |\text{MPE}|$

UUC = Unit Under Calibration

Fail = $|\text{error}| + |\text{uncertainty}| > |\text{MPE}|$

MPE = Maximum Permissible Error

Description of UUC : Range pH -2 to pH 16

Condition As-Received : Used Item

The measurement results and statements of conformity with specification only relate to the item calibrated.

Certified Reference Material & Traceability of Certificate :

The International System of Units (SI) through

- NIMT Lot No. 040822_2 for pH 4.003 Buffer Solution, Due 20 NOV 2024
- CPA chem Lot No. 1008799 for pH 7.0 Buffer Solution, Due 10 JUL 2026
- NIMT Lot No. 230822_2 for pH 10.01 Buffer Solution, Due 20 NOV 2024

End of Certificate

Page 2 of 2



รับรองสำเนาถูกต้อง
ผู้จัดการฝ่ายควบคุมคุณภาพ



SCIMET Co., Ltd.
1194 Soi Wachirathamsathit 57, Bangchak,
Phrakhanong, Bangkok 10260 Thailand
Email:scimet2022@gmail.com, Tel: 02 460 9239
https://www.scimet.co.th



Certificate No. C17240307

Calibration Certificate

Equipment:	Cooled Incubator	Job No.:	KSMT2402653
Model:	BIC-140	Received Date:	27 September 2024
Serial No.(or ID):	100613-1 (ELABBODC140NO1)	Issued Date:	30 September 2024
Manufacturer:	M-LAB	Page:	1 of 3
Condition:	In Condition		
Ventilation Valve:	None	Shelves(pc.):	5

Customer

Envilab Co., Ltd.
540, 540/1 Soi Bangkhuae 7, Bangkhuae, Bangkhuae, Bangkok 10160

Calibration Place

Envilab Co., Ltd. (B300 CH1 ROOM)
540, 540/1 Soi Bangkhuae 7, Bangkhuae, Bangkhuae, Bangkok 10160

Calibration Date

27 September 2024

Environment Condition

Temperature: 20.8 °C \pm 1.0 °C
Humidity: 54.8 %RH \pm 2.6 %RH

The Method used

In-house method, WI17, based on TLAS-G20

Traceability

This certificate is traceable to the SI Units maintained by National Institute of Metrology (NIMT), Thailand through SCIMET Co.,Ltd.Certificate No. C23240083

This certificate is issued the units of measurement according to the International System of Units (SI). It provides traceability of measurement to international or national standard or other recognized national standard laboratories.

The measurement uncertainty stated is the expanded uncertainty which is obtained from the standard uncertainty multiplied by the coverage factor ($k=2$) to provide a level of confidence of approximately 95%. It is determined in accordance with the Guide to Expression of Uncertainty in Measurement (GUM).

These results may be affected by deviations from specified conditions. The results relate only to the items tested, calibrated or sampled. The report shall not be reproduced except in full without approval of SCIMET Co., Ltd.

(Mongkolwat Hasanon)
Person in charge




(Mr. Thalerngkeat Pounngam)
Authorized signatory



รับรองสำเนาถูกต้อง
ผู้จัดการฝ่ายควบคุมคุณภาพ

FC17-02: 30 MAY 2023

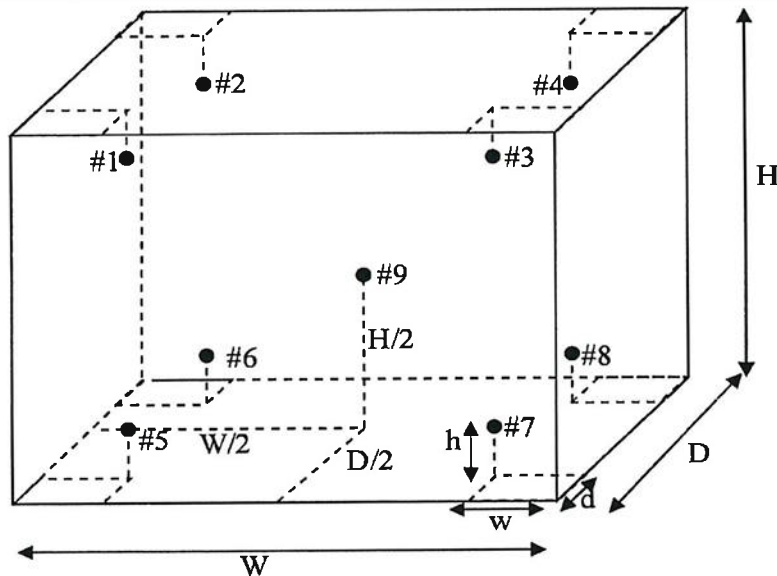

Standard Installation Locations

Volume (Calibration Zone)= 58 (Liters)

Inside chamber: W = 38 (cm) D = 32 (cm) H = 114 (cm)

Standard Locations (#1, #2, #3, #4): w = 5 (cm) d = 5 (cm) h = 10 (cm)

Standard Locations (#5, #6, #7, #8): w = 5 (cm) d = 5 (cm) h = 10 (cm)

#9: Geometric center of the chamber

Position of Std	#1	#2	#3	#4	#5	#6	#7	#8	#9
Channel of Logger	201	202	203	204	205	206	207	208	209

Definitions

Indicating Temperature: The average reading of indicating device which forms the integral part of the enclosure.

Measured Temperature: The average reading of standards at any positions or location.

Measured Uniformity: The maximum difference of measured temperatures between of any probes and the measured temperature at the reference location which are observed at same time or at close observation time as possible to determine the temperature pattern or homogeneity with the chamber at steady-state. The reference probe is preferably located in the geometric center of the chamber.

Measured Stability: The one-half of greatest maximum difference of measured temperatures at any one probe.

Overall Variation: The difference of maximum and minimum measured temperatures throughout observation time.

บริษัท ชายนีเมก จำกัด (SCIMET CO., LTD.)

1194 Soi Wachirathamsathit 57, Bangchak, Phrakhanong, Bangkok 10260 Thailand
Email: scimet2022@gmail.com, Tel: 02 460 9239



รับรองสำเนาถูกต้อง
ผู้จัดการฝ่ายควบคุมคุณภาพ

FC17-02: 30 MAY 2023

Calibration Results:

Without adjustment

Measurement Temperature at Spread Locations, Indicating of Unit Under Calibration: 20.0 °C

Locations	Measured Temperature (°C)	Correction (°C)	Uncertainty (± °C)
#1	19.54	-0.46	0.38
#2	19.49	-0.51	0.39
#3	19.87	-0.13	0.39
#4	20.04	0.04	0.37
#5	20.36	0.36	0.36
#6	20.21	0.21	0.37
#7	20.10	0.10	0.36
#8	20.19	0.19	0.37
#9	20.48	0.48	0.35

Temperature Distribution

Desired (°C)	Setting (°C)	Indicating (°C)	Measured Temperature at Spread Locations (°C)									Uncertainty (± °C)*
			#1	#2	#3	#4	#5	#6	#7	#8	#9	
20.0	20.0	20.0	19.54	19.49	19.87	20.04	20.36	20.21	20.10	20.19	20.48	0.39

Chamber Characterization

Indicating (°C)	Measured Uniformity (°C)	Measured Stability (± °C)	Overall Variation (°C)
20.0	1.07	0.18	1.26

Note: * Maximum uncertainty of the each position

The End of Certificate

Statements of conformity:

This conformity certificate documents the validity of the following statements of conformity based on the measurement results of corresponding calibration certificate:

The correction of indication determined during calibration are under given measurement and environmental conditions and considering the expanded measurement uncertainty (coverage probability 95%) within the specification. The given measurement uncertainty already includes other all effects by according to the standard method, TLAS-G20. Therefore, those parameters have not

Tolerance and Decision rules:

Assessment of the conformity of the measurement device are done based on direct comparison of the relevant measurement results with the tolerances and decision rule are prescribed by the customer.

- Decision rule :** ☐ Choice A Binary Statement for Simple Acceptance Rule ($w = 0$), Specific Risk $< 50\%$ PFA.
- ☒ Choice B Non-binary statement with guard band ($w = 1$ U), Pass or Fail Specific Risk $< 2.5\%$ PFA and Condition Pass or Condition Fail Specific Risk $< 50\%$ PFA.
- ☐ Choice C Customer defined, Customers may define arbitrary multiple of r to have applied as guard band ($w = r$ U) .
- ; PFA: Probability of False Accept




(Mr. Thalerngkeat Pongngam)
Authorized signatory

Without adjustment

Desired Temperature : 20.0°C

Tolerances : 1.0 °C

Measurement Temperature at Spread Locations, Indicating of Unit Under Calibration: 20.0 °C

Locations	Measured (°C)	Correction of UUC. (°C)	Guard band (W) (± °C)	Tolerance (± °C)	Conformity
#1	19.54	-0.46	0.38	1.0	Pass
#2	19.49	-0.51	0.39	1.0	Pass
#3	19.87	-0.13	0.39	1.0	Pass
#4	20.04	0.04	0.37	1.0	Pass
#5	20.36	0.36	0.36	1.0	Pass
#6	20.21	0.21	0.37	1.0	Pass
#7	20.10	0.10	0.36	1.0	Pass
#8	20.19	0.19	0.37	1.0	Pass
#9	20.48	0.48	0.35	1.0	Pass

Correction of UUC.* = Measured Temperature - Desired Temperature

The validity of the statements of conformity cannot be guaranteed for different places of use, environmental conditions or improper use.

The End of Statements of Conformity

บริษัท ชายนันท์ จำกัด (SCIMET CO., LTD.)

1194 Soi Wachirathamsathit 57, Bangchak, Phrakhanong, Bangkok 10260 Thailand
Email: scimet2022@gmail.com, Tel: 02 460 9239



รับรองสำเนาถูกต้อง
ผู้จัดการฝ่ายควบคุมคุณภาพ


FC17-02: 30 MAY 2023

Corr_Distribution & Max_Measurement Uncertainty

Job_No. KSMT2402653

Without adjustment

Correction (°C)

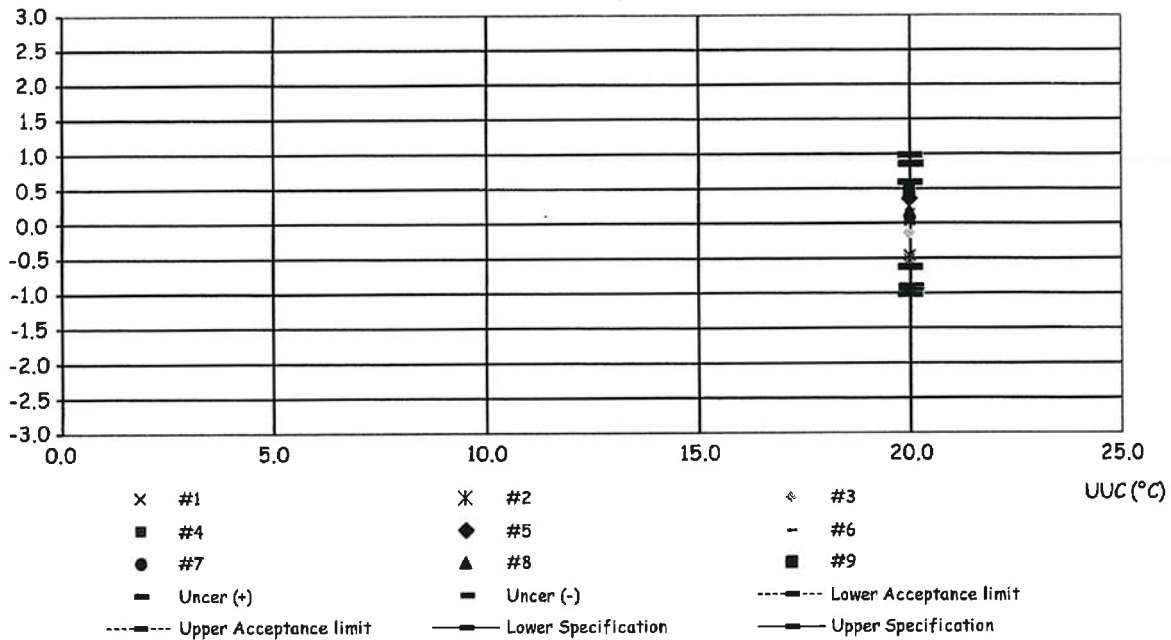


Temperature Distribution @ 20.0°C

Job_No. KSMT2402653

Without adjustment

Std(°C)

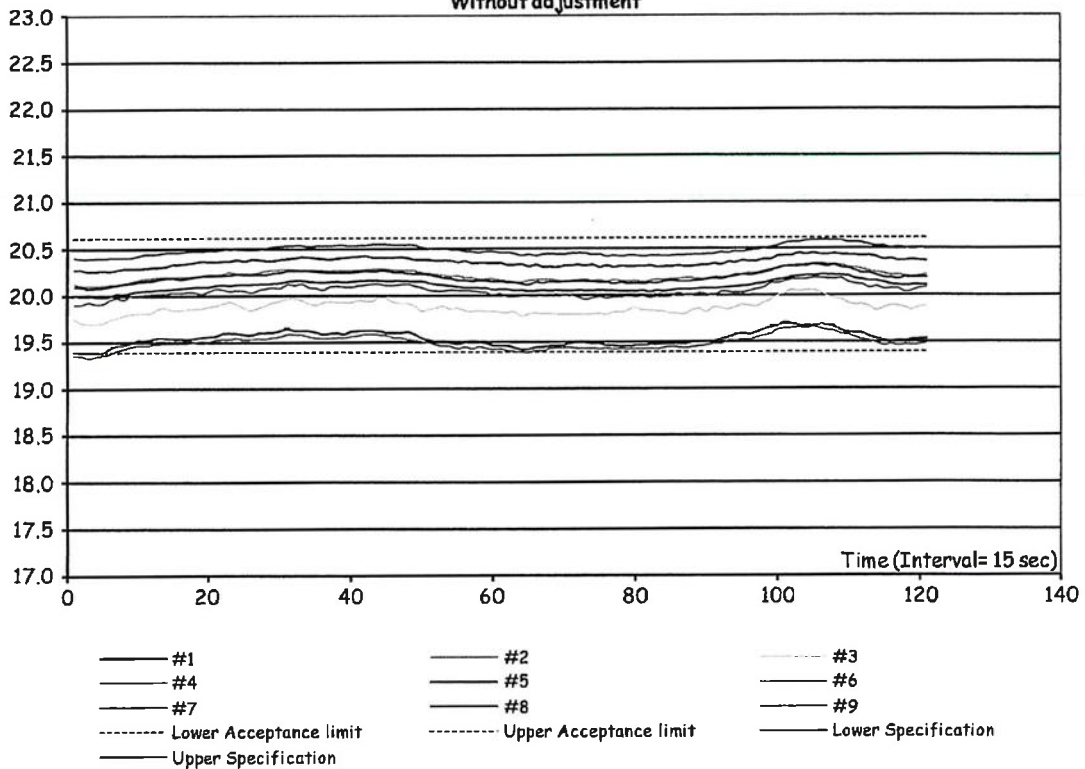

Envilab Co.,Ltd.

รับรองสำเนาถูกต้อง
ผู้จัดการฝ่ายควบคุมคุณภาพ



ใบตรวจสอบสภาพเครื่องควบคุมอุณหภูมิ

เลขที่ใบงาน: KSMT2402653

ชนิดเครื่องมือ: Cooled Incubator

รุ่น: BIC-140

หมายเลขเครื่อง: 100613-1 (ELABBODC140NO1)

ตรวจสอบ (รับ)		รายการตรวจเช็ค	ตรวจสอบ (ส่ง)		หมายเหตุ
27 Sep 2024			27 Sep 2024		
ปกติ	ไม่ปกติ		ปกติ	ไม่ปกติ	
		General			
<input checked="" type="checkbox"/>	<input type="checkbox"/>	1. สายไฟ	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	2. การทำงาน Main Switch	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	3. การทำงาน Selector Key	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	4. การแสดงผล Display	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	5. การทำงาน พัดลม	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input type="checkbox"/>	<input type="checkbox"/>	6. สภาพ Lever of Ventilation valve	<input type="checkbox"/>	<input type="checkbox"/>	-
<input checked="" type="checkbox"/>	<input type="checkbox"/>	7. สภาพ Lever door open / close	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	8. สภาพ Door seal	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	9. การทำงานของระบบ Safety	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	10. การทำงานของระบบทำความเย็น	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input type="checkbox"/>	<input type="checkbox"/>	11. การทำงานของระบบทำความชื้น	<input type="checkbox"/>	<input type="checkbox"/>	-
<input checked="" type="checkbox"/>	<input type="checkbox"/>	12. สภาพตัวเครื่อง	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	13. สภาพแวดล้อม ณ สถานที่ตั้งเครื่อง	<input checked="" type="checkbox"/>	<input type="checkbox"/>	

ข้อแนะนำ :

Mr. Mongkolwat Hasanon

Service Engineer

บริษัท ชายนันเมก จำกัด (SCIMET CO., LTD.)

1194 Soi Wachirathamsathit 57, Bangchak, Phrakhanong, Bangkok 10260 Thailand
Email: scimet2022@gmail.com, Tel: 02 460 9239



รับรองสำเนาถูกต้อง
ผู้จัดการฝ่ายควบคุมคุณภาพ

FI17-00: 08 MAR 2023



SCIMET Co., Ltd.
1194 Soi Wachirathamsathit 57, Bangchak,
Phrakhanong, Bangkok 10260 Thailand
Email:scimet2022@gmail.com, Tel:095-552-4939

Certificate No. C27240001

Calibration Certificate

Equipment: DO METER
Model: HI9147
Serial No.(or ID): H00007030
Manufacturer: HANNA
Condition: In Condition

Job No.: KSMT2400445
Received Date: 04 March 2024
Issued Date: 14 March 2024
Page: 1 of 2

Customer

Envilab Co., Ltd.
540, 540/1 Soi Bangkhuae 7, Bangkhuae, Bangkhuae, Bangkok 10160

Calibration Place

Environment Laboratory, SCIMET Co., Ltd.
1194 Soi Wachirathamsathit 57, Bangchak, Prakhnong, Bangkok 10260 Thailand

Calibration Date

14 March 2024

Environment Condition

Temperature: 23 °C \pm 2 °C
Humidity: 50 %RH \pm 15 %RH

The Method used

In-house method, WI27 , By comparison with certified
dissolved oxygen solution standard

Traceability

This is certificate is traceable to SI Units , Sample test and
temperature test are assured through HANNA instruments
company certificare No. 29E31, through Quality Reborn
Co.,LTD certificare No.QR23-1169

This certificate is issued the units of
measurement according to the International
System of Units (SI). It provides traceability
of measurement to international or national
standard or other recognized national
standard laboratories.

The measurement uncertainty stated is
the expanded uncertainty which is obtained
from the standard uncertainty multiplied by
the coverage factor ($k=2$) to provide a level
of confidence of approximately 95%. It is
determined in accordance with the Guide to
Expression of Uncertainty in Measurement
(GUM).

These results may be affected by
deviations from specified conditions. The
results relate only to the items tested,
calibrated or sampled. The report shall not be
reproduced except in full without approval of
SCIMET Co., Ltd.

Mr.Dumrong Boonsopon
Person in charge



บริษัท ชัยนิเทศ จำกัด



รับรองสำเนาถูกต้อง
ผู้จัดการฝ่ายควบคุมคุณภาพ

Mr. Thalerngkeat Pongngarm
Authorized signatory

Calibration Results:

Electrode Serial No. KC3N05V1R
Model : H176409
Brand : HANNA

Electrode Test

Atmospheric pressure measured while calibrating. 755.54 mmHg
Temperature measured while calibrating. (± 0.2 °C) 25.0 °C
The Oxygen Solubility was calculated from the ambient conditions. 8.21 \pm 0.03 mg/L
The Oxygen Solubility reading from the DO METER 8.23 mg/L

Sample Test

Standard Oxygen Solution	Unit Under Calibration Reading	Correction	Coverage Factor (k)	Uncertainty of Measurement (\pm)
0.00 mg/L	0.00 mg/L	0.000 mg/L	2.00	0.13 mg/L

Temperature Electrode

Dimension of Probe;

Length : 140 mn.
Diameter : 21 mn.
Immersion Depth 80 mn.

STD. Reading (°C)	UUC. Reading (°C)	Correction of UUC (°C)	Coverage Factor (k)	Uncertainty of Measurement (\pm °C)
25.01	25.0	0.01	2.00	0.15

The End of Certificate



รับรองสำเนาถูกต้อง
ผู้จัดการฝ่ายควบคุมคุณภาพ

บริษัท ชายนีเมท จำกัด (SCIMET CO., LTD.)

1194 Soi Wachirathamsathit 57, Bangchak, Phrakhanong, Bangkok 10260 Thailand
Email: scimet2022@gmail.com, Tel: 095 552 4939



ใบตรวจสอบสภาพเครื่อง Do Meter

เลขที่ใบงาน: KSMT2400445

ชนิดเครื่องมือ: DO METER

รุ่น: HI9147

หมายเลขเครื่อง: H00007030

ตรวจสอบ (รับ)		รายการตรวจเช็ค	ตรวจสอบ (ส่ง)		หมายเหตุ
14 Mar 2024			14 Mar 2024		
ปกติ	ไม่ปกติ		ปกติ	ไม่ปกติ	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	1. ความสมบูรณ์เครื่อง	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	2. ความสะอาด (ช่องใส่ตัวอย่าง, ภายใน-นอกเครื่อง)	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	3. สวิทช์ ปิด – เปิด เครื่อง (On-Off Swicth)	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	4. ปุ่มกด (Keypad)	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	5. หน้าจอ (Display, Screen Contrast)	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	6. อิเล็กโทรด (Electrode and Connection Cable)	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	7. สายอิเล็กโทรด	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	8. เซ็นเซอร์อิเล็กโทรด	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	9. ขาจับอิเล็กโทรด (Stand)	<input checked="" type="checkbox"/>	<input type="checkbox"/>	

ข้อแนะนำ :

Mr.Dumrong Boonsopon

Service Engineer



รับรองสำเนาถูกต้อง
ผู้จัดการฝ่ายควบคุมคุณภาพ

บริษัท ชายนีเมก จำกัด (SCIMET CO., LTD.)

1194 Soi Wachirathamsathit 57, Bangchak, Phrakhanong, Bangkok 10260 Thailand
Email: scimet2022@gmail.com, Tel: 095 552 4939

CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhaphrachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech_cal@yahoo.com, calibratech_cal@hotmail.com



NSC-TISI-TIS17025
CALIBRATION 0030

Certificate of Calibration

Certificate No. : 67-400166-2

Page : 1 of 2

Submitted by : Envilab Co., Ltd.
540, 540/1 Soi Bangkhae 7, Bangkhae, Bangkok 10160

Equipment : Water Bath
Manufacturer : Memmert Model : WNB 14
Range : N/A °C Resolution : 0.1 °C
Serial No. : L412.2222 ID No. : ELABWBWNB29N01

Environment : On site calibration was carried out at the Laboratory, Envilab Co., Ltd.

Ambient Temperature : (29.0 to 30.0) °C

Relative Humidity : (60 to 65) %

Line Voltage : (224.2 to 225.2) V

Date of Received : 20 March 2024

Date of Calibration : 20 March 2024

Date of Issue : 22 March 2024

Calibrated by : Kittisak Kokaeo

Calibration Method : This instrument was calibrated by In-house method CAL-M4006 based on ASTM E715-80
The temperature scale used was based on ITS-90

Reference Standard Instruments : This certification is traceable to the International System of Units
Standard Digital Thermometer with RTD probe

<u>ID No.</u>	<u>Cert. No.</u>	<u>Due Date</u>	<u>Traceability</u>
400046 & 400024	66-400547-2	02 Apr 2024	National Institute of Metrology Thailand (NIMT)



รับรองสำเนาถูกต้อง
ผู้จัดการฝ่ายควบคุมคุณภาพ

Approved by :

(Surachai Promthong)

Laboratory Manager

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhprachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech.cal@yahoo.com, calibratech.cal@hotmail.com

Certificate of Calibration


Certificate No. :67-400166-2

Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Function : Temperature measurement

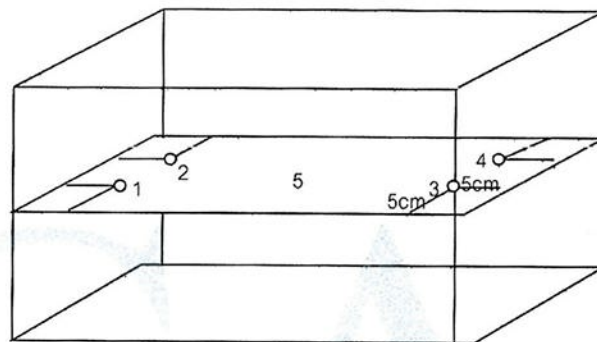

Front

Test Point (° C)	Setting Temperature (° C)	Indicating Temperature (° C)	Measured Temperature (° C) @ Sensor No.					Uncertainty (± ° C)	Measured Uniformity (° C)	Measured Stability (° C)
			1	2	3	4	5			
95.0	94.5	94.5	95.12	95.18	95.11	95.02	95.17	0.23	0.26	0.12

Remark The uncertainty is not combine uniformity of the water bath

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

- o0o -



Envilab Co.,Ltd.

รับรองสำเนาถูกต้อง
ผู้จัดการฝ่ายควบคุมคุณภาพ

[Signature]



Certificate of Calibration

Certificate No. : 67-400166-1

Page : 1 of 2

Submitted by : Envilab Co., Ltd.
540, 540/1 Soi Bangkhae 7, Bangkhae, Bangkok 10160

Equipment : Temperature controlled enclosure (Oven)
Manufacturer : Memmert Model : UF 75
Range : N/A °C Resolution : 0.1 °C
Serial No. : B319.0600 ID No. : ELABHAOVEN0600

Environment : On site calibration was carried out at the Laboratory, Envilab Co., Ltd.
Ambient Temperature : (29.0 to 30.0) °C
Relative Humidity : (60 to 650) %
Line Voltage : (224.2 to 225.2) V

Date of Received : 20 March 2024

Date of Calibration : 20 March 2024

Date of Issue : 22 March 2024

Calibrated by : Kittisak Kokaeo

Calibration Method : CAL-M4004, TLAS G-20

The temperature scale used was based on ITS-90

Reference Standard Instruments : This certification is traceable to the International System of Units

Standard Digital Thermometer with Thermocouple probe

ID No.	Cert. No.	Due Date	Traceability
400046 & 400028	66-400547-3	05 Apr 2024	National Institute of Metrology Thailand (NIMT)



รับรองสำเนาถูกต้อง
ผู้จัดการฝ่ายควบคุมคุณภาพ

Approved by :

(Surachai Promthong)

Laboratory Manager

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 67-400166-1


Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Function : Temperature measurement

This instrument was setting air ventilation at position 0 (close)

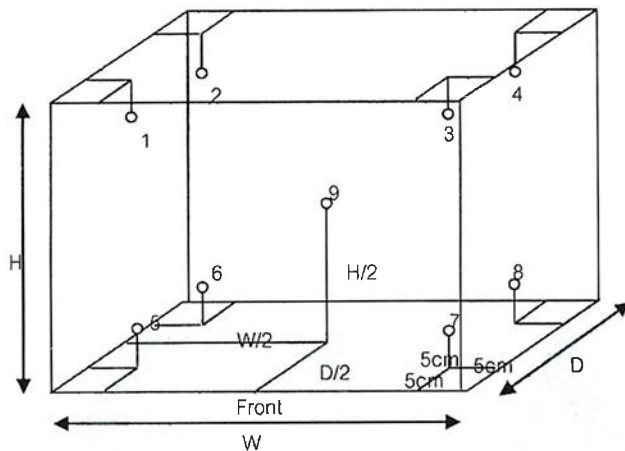

Inside of Chamber

W = 0.40 m

D = 0.33 m

H = 0.56 m

Capacity = 0.07 m³

Test Point (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Temperature (°C) @ Sensor No.									Uncertainty (± °C)
			1	2	3	4	5	6	7	8	9	
104.0	103.5	103.5	104.1	104.4	104.1	104.3	104.1	104.0	104.0	103.7	104.3	0.70
110.0	109.5	109.5	110.1	110.4	110.1	110.3	110.2	110.1	110.1	109.4	110.3	0.72
180.0	179.0	179.0	179.5	180.9	180.3	180.6	180.5	180.3	180.2	180.2	180.8	0.95

Test Point (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Uniformity (°C)	Measured Stability (°C)	Overall Variation (°C)
104.0	103.5	103.5	0.7	0.1	1.0
110.0	109.5	109.5	1.1	0.1	1.2
180.0	179.0	179.0	1.5	0.2	1.6

Remark The uncertainty is not combine uniformity of the air chamber

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

- ๐0๐ -



Enviab Co.,Ltd.

รับรองสำเนาถูกต้อง
ผู้จัดการฝ่ายควบคุมคุณภาพ



CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhaphrachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech-cal@yahoo.com, calibratech-cal@hotmail.com



Certificate of Calibration

Certificate No. : 67-200060-2

Page : 1 of 2

Submitted by : Envilab Co., Ltd.
540, 540/1 Soi Bangkhae7, Bangkhae, Bangkok 10160

Equipment : Electronic Balance
Manufacturer : METTLER TOLEDO **Model :** XSR205DU
Serial No. : B911363567 **ID No. :** ELABBALANCEN06
Capacity : 220 g **Resolution :** 0.00001g/81g, 0.0001g/220g

Environment : On site calibration was carried out at the B304 Balance Room, Envilab Co., Ltd.
Ambient Temperature : (20.0 to 20.5) °C
Relative Humidity : (54.2 to 59.1) %
Air Pressure : 1013.0 mbar

Date of Received : 20 February 2024

Date of Calibration : 20 February 2024

Date of Issue : 21 February 2024

Calibrated by : Satja Sangkhum

Calibration Method : In-house method CAL-M2001 based on UKAS Publication ref : LAB 14
Edition 7 - November 2022

Reference Standard Instruments : This certification is traceable to the International System of Units

Standard Weights

<u>ID No.</u>	<u>Cert. No.</u>	<u>Due Date</u>	<u>Traceability</u>
E261-E2624	C02232088	08 Nov 2024	National Institute of Metrology (Thailand), (NIMT)



รับรองสำเนาถูกต้อง
ผู้จัดการฝ่ายควบคุมคุณภาพ

Approved by :

(Surachai Promthong)

Laboratory Manager

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhaprachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech.cal@yahoo.com, calibratech.cal@hotmail.com

Certificate of Calibration

Certificate No. : 67-200060-2

Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Departure of indication from nominal value


Nominal Value (g)	Correction (g)	Uncertainty \pm (g)
0.1	0.00000	0.000015
0.5	0.00001	0.000022
1	0.00000	0.000026
2	0.00001	0.000034
5	-0.00001	0.000043
10	0.00000	0.000053
50	0.00003	0.00011
100	0.0001	0.00020
150	0.0001	0.00038
200	0.0002	0.00038

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2.00$,
providing a level of confidence of approximately 95%

Eccentric error

Load test : 50 g
A B C D E
0.00000 0.00000 0.00010 0.00000 0.00000 g



Repeatability

Load test : 200 g
Stdev. : 0.000032 g

- o0o -



Envilab Co.,Ltd.

รับรองสำเนาถูกต้อง
ผู้จัดการฝ่ายควบคุมคุณภาพ



CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhprachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech.cal@yahoo.com, calibratech.cal@hotmail.com



Certificate of Calibration

Certificate No. : 67-300147-11

Page : 1 of 2

Submitted by : Envilab Co.,Ltd.

540, 540/1 Soi Bangkhac 7, Bangkhac, Bangkok 10160

Equipment : Measuring Pipette

Manufacturer : Witeg

Class : A

Capacity : 25 ml

Graduation : 0.1 ml

ID No. : G-HM-013/23

Environment : Ambient Temperature : (20 ± 3) °C

Relative Humidity : (50 ± 10) %

Air Pressure : 1006.8 mbar.

Date of Received : 13 March 2024

Date of Calibration : 19 March 2024

Date of Issue : 19 March 2024

Calibrated by : Arcerat Sombun

Calibration Method : In-house method CAL-M3001 based on ASTM E 542-22

Reference Standard Instruments : This certification is traceable to the International System of Units

Electronic Balance

<u>ID No.</u>	<u>Cert. No.</u>	<u>Due Date</u>	<u>Traceability</u>
241005	66-200388-4	02 Jun 2024	National Institute of Metrology (Thailand) (NIMT)

Approved by :

(Wipa Tovadec)

Supervisor



รับรองสำเนาถูกต้อง
ผู้จัดการฝ่ายควบคุมคุณภาพ

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhprachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech-cal@yahoo.com, calibratech-cal@hotmail.com

Certificate of Calibration

Certificate No. : 67-300147-11

Page : 2 of 2

Result of Calibration : This result of true Volume is referred to standard temperature at 20 °C

UUC Condition As-Received : Good

Delivery Time : 14.28 sec.

Nominal Volume (ml)	Measuring Volume (ml)
1	1.0304
10	9.9852
25	24.9764

Uncertainty of measurement with in \pm 0.0067 ml

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2.00$,
providing a level of confidence of approximately 95%

- o0o -



Envilab Co.,Ltd.

รับรองสำเนาถูกต้อง
ผู้จัดการฝ่ายควบคุมคุณภาพ





MIRACLE INTERNATIONAL TECHNOLOGY CO.,LTD

214 Bangwack Rd. Bangpai Bangkhae Bangkok 10160
Tel.: 0-2865-4647-8 Fax: 0-2865-4649 <http://www.mit.in.th>



CALIBRATION CERTIFICATE

Certificate No. : S2024040558-0002

Date Issued : 03-May-24

Customer : Envilab Co., Ltd.
540, 540/1 Soi Bangkhae 7, Bangkhae, Bangkok, Thailand
10160

Equipment : Lab Refrigerator (TMF-PLR221)

Manufacturer : Thermo Scientific

Model : PLR221

Serial No. : 2210M319042801

ID No./Tag No. : ELABREFRIGEN02

Date Received : 02-May-24

Date Calibrated : 02-May-24

Calibrated by : Mr. Varuch Jearrajinda

Calibration Method or Calibration Procedure Used

Standard method : CP-05 TLAS G-20.

This certificate is traceable to national standards, which realize the units of measurement according to the International System of Units (SI).

Result of Calibration

The reported uncertainty of measurement was based on standard uncertainty multiplied by a coverage factor $k = 2$, providing a level confidence approximately 95 percent.

This certificate may not be reproduced other than in full except with the prior written approval of the Miracle International Technology Company Limited.

Approved by:

Sarayuth T.
(Mr. Sarayuth Tochua)



Page 1 of 2



รับรองสำเนาถูกต้อง
ผู้จัดการฝ่ายควบคุมคุณภาพ

Certificate No. : S2024040558-0002

Environment : Ambient Temperature : Start record 26.6 °C, Stop record 26.8 °C
Relative Humidity : Start record 54.1 %RH, Stop record 54.5 %RH

Calibration Temperature (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Stability ¹ (°C)	Measured Uniformity ² (°C)	Overall Variation ³ (°C)
4	4	4	0.88	0.69	1.94

Without adjustment

Calibration Temperature (°C)	STD No. 1 (°C)	STD No. 2 (°C)	STD No. 3 (°C)	STD No. 4 (°C)	STD No. 5 (°C)	STD No. 6 (°C)	STD No. 7 (°C)	STD No. 8 (°C)	STD No. 9 (°C)	Uncertainty ⁴ ±°C
4	4.23	4.35	4.44	4.46	4.35	4.24	4.34	3.96	4.13	1.2

Decision Rule with Guard Band

Calibration Temperature (°C)	No. 1	No. 2	No. 3	No. 4	No. 5	No. 6	No. 7	No. 8	No. 9	MPE (±°C)
4	Pass	Pass	Pass	Pass	Pass	Pass	Pass	Pass	Pass	2


Pass = |error| + |uncertainty| ≤ |MPE|

MPE = Maximum Permissible Error

Fail = |error| + |uncertainty| > |MPE|

Note : Probe No. 9 is Reference Probe

Setting Air Fresh No. 0



Condition As-Received : Used Item

The measurement results and statements of conformity with specification only relate to the item calibrated.

Measurement Standards Used & Traceability :

The International System of Units (SI) through

MIT Certificate No. L202403007-0012 for Digital Thermometer with Probe (Agilent) Module 1 (93) Serial No. MY41008700, Due 10-Sep-24

Notes : 1. The temperature stability is the one-half of greatest maximum difference of measured temperatures at any one probe.

2. The temperature uniformity is the maximum difference of measured temperatures between of any probes and the measured temperature at the reference location which are observed at same time.

3. Overall variation is the difference of maximum and minimum measured temperatures throughout observation time.

4. The uncertainty of measurement is included temperature stability.

5. The temperature uniformity, stability, overall variation and indicating temperature is applicable to all air or gas filled temperature controlled enclosures at atmospheric pressure.

End of Certificate



Envilab Co., Ltd.

Page 2 of 2

รับรองสำเนาถูกต้อง
ผู้จัดการฝ่ายควบคุมคุณภาพ

CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhaprachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech-cal@yahoo.com, calibratech-cal@hotmail.com



NSC-TISI-TIS17025
CALIBRATION 0030

Certificate of Calibration

Certificate No. : 67-300147-2

Page : 1 of 2

Submitted by : Envilab Co.,Ltd.

540, 540/1 Soi Bangkhae 7, Bangkhae, Bangkok 10160

Equipment : Cylinder

Manufacturer : PYREX

Class : A

Capacity : 50 ml

Graduation : 1 ml

ID No. : C-WW-011/23

Environment : Ambient Temperature : (20 ± 3) °C

Relative Humidity : (50 ± 10) %

Air Pressure : 1009.4 mbar.

Date of Received : 13 March 2024

Date of Calibration : 19 March 2024

Date of Issue : 19 March 2024

Calibrated by : Arcerat Sombun

Calibration Method : In-house method CAL-M3001 based on ASTM E 542-22

Reference Standard Instruments : This certification is traceable to the International System of Units

Electronic Balance

ID No.	Cert. No.	Due Date	Traceability
241002	66-200388-1	02 Jun 2024	National Institute of Metrology (Thailand) (NIMT)

Approved by :

(Wipa Tovadce)

Supervisor



รับรองสำเนาถูกต้อง
ผู้จัดการฝ่ายควบคุมคุณภาพ

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhaprachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech_cal@yahoo.com, calibratech_cal@hotmail.com

Certificate of Calibration

Certificate No. : 67-300147-2

Page : 2 of 2

Result of Calibration : This result of true Volume is referred to standard temperature at 20 °C

UUC Condition As-Received : Good

Nominal Volume (ml)	Measuring Volume (ml)
30	29.69
50	49.87

Uncertainty of measurement with in \pm 0.054 ml

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2.00$,
providing a level of confidence of approximately 95%

- o0o -



Envilab Co.,Ltd.

รับรองสำเนาถูกต้อง
ผู้จัดการฝ่ายควบคุมคุณภาพ



CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhprachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech.cal@yahoo.com, calibratech.cal@hotmail.com



Certificate of Calibration

Certificate No. : 67-300147-2

Page : 1 of 2

Submitted by : Envilab Co.,Ltd.

540, 540/1 Soi Bangkhac 7, Bangkhac, Bangkok 10160

Equipment : Cylinder

Manufacturer : PYREX

Class : A

Capacity : 50 ml

Graduation : 1 ml

ID No. : C-WW-011/23

Environment : Ambient Temperature : (20 ± 3) °C

Relative Humidity : (50 ± 10) %

Air Pressure : 1009.4 mbar.

Date of Received : 13 March 2024

Date of Calibration : 19 March 2024

Date of Issue : 19 March 2024

Calibrated by : Arcerat Sombun

Calibration Method : In-house method CAL-M3001 based on ASTM E 542-22

Reference Standard Instruments : This certification is traceable to the International System of Units

Electronic Balance

<u>ID No.</u>	<u>Cert. No.</u>	<u>Due Date</u>	<u>Traceability</u>
241002	66-200388-1	02 Jun 2024	National Institute of Metrology (Thailand) (NIMT)

Approved by :

(Wipa Tovadce)

Supervisor



รับรองสำเนาถูกต้อง
ผู้จัดการฝ่ายควบคุมคุณภาพ

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhprachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech.cal@yahoo.com, calibratech.cal@hotmail.com

Certificate of Calibration

Certificate No. : 67-300147-2

Page : 2 of 2

Result of Calibration : This result of true Volume is referred to standard temperature at 20 °C

UUC Condition As-Received : Good

Nominal Volume (ml)	Measuring Volume (ml)
30	29.69
50	49.87

Uncertainty of measurement with in \pm 0.054 ml

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2.00$,
providing a level of confidence of approximately 95%

- o0o -



Envilab Co.,Ltd.

รับรองสำเนาถูกต้อง

ผู้จัดการฝ่ายควบคุมคุณภาพ

