

Certificate of Calibration

Certificate No. : 67-400561-3

Page : 1 of 2

Submitted by : Ecotech Water Co., Ltd.

20 Soi Kheharomklao 74 Yaek 6, Ratphatthana, Saphansung, Bangkok 10240

Equipment : Autoclave

Manufacturer : Labtech

Model : LAC-5060S

Range : N/A °C

Resolution 0.1 °C

Serial No. : 090414007

ID No. : INS008

Environment : On site calibration was carried out at the Laboratory, Ecotech Water Co., Ltd.

Ambient Temperature : (25.5 to 26.0) °C

Relative Humidity : (50 to 55) %

Line Voltage : (225.0 to 226.5) V

Date of Received : 28 September 2024

Date of Calibration : 28 September 2024

Date of Issue : 02 October 2024

Calibrated by : Permpon Chanpu

Calibration Method : This instrument was calibrated by In-house method CAL-M4007 based on BS 2646 Part 1 : 2021

The temperature scale used was based on ITS-90

Reference Standard Instruments : This certification is traceable to the International System of Units

Standard Temperature Data Logger with RTD pt 100

ID No.	Cert. No.	Due Date	Traceability
400039	67-400356-1	28 Dec 2024	National Institute of Metrology Thailand (NIMT)
400040	67-400356-2	28 Dec 2024	National Institute of Metrology Thailand (NIMT)
400041	67-400356-3	28 Dec 2024	National Institute of Metrology Thailand (NIMT)

Approved by :



(Permpon Chanpu)

Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration


Certificate No. 67-400561-3

Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Function : Temperature measurement

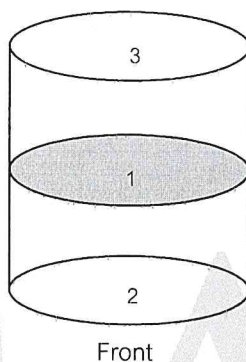

Test Point (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Temperature (°C) @ Sensor No.			Uncertainty (± °C)	Measured Uniformity (°C)	Measured Stability (°C)	Sterilizing Time (minute)	Pressure Gauge Reading (kgf/cm²)
			1	2	3					
121.0	121.0	121.0	121.4	121.4	121.4	0.71	0.1	0.2	15	1.2

Remark

1. UUC : Unit Under Calibration
2. Pressure Gauge reading are out of accreditation's scope.

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

- o0o -

[Handwritten signature]



Certificate No. : HIT-2446-1899

Page : 1 of 2

CERTIFICATE OF CALIBRATION

Equipment : Dissolved Oxygen and BOD Meter

Meter Model : HI98193 **Serial No. :** 07470053101

Probe Model : HI764073 **Serial No. :** KC1N53G5T

Manufacturer : Hanna Instruments **Made in :** Romania

Condition As-Received : Used Product **Reference :** RE242195

Ambient Temperature : $(25 \pm 2)^{\circ}\text{C}$ **Relative Humidity :** $(50 \pm 15)\% \text{ RH}$

Customer name : Ecotech Water Systems Co., Ltd.
20 Soi Khaharomklao 74 Yaek 6, Ratphatthana,
Saphansung, Bangkok 10240

Received date : 11 November 2024


Calibrate date : 14 November 2024

Issue date : 15 November 2024

Calibrated Location : Hanna Instruments (Thailand) Ltd.

Calibration Procedure : This calibrator was conducted by using in-house: calibration procedure
CP-11 by using certified reference material (CRM).

Calibrated by : ☒ Mr. Pichit Petthong
☐ Mr. Channarong Soinak

Approved by : 
Mr. Anan Suwanchaisakul
Authorized Signatory

This certificate was certified only for the instrument we calibrated.

This result of calibration was found accurate on date and place of calibration only.

** This certificate may not be reproduced other than in full, except with the prior written **

approval of the head of Hanna Instrument (Thailand)

Condition of this calibration result

1. Reference Standard Instruments : This certification is traceable to the international unit of thru Technology Promotion Association (Thailand-Japan).

Instruments	Model	Serial No.	Certificate No.
Thermometer with sensor	HI98509	39643D	24T1281
Digital Thermo-Hygrometer	HT-771SD	AI.07155	24H41

2. Reference Standard Materials : DO calibration standard traceable to Hanna Instrument Ltd.

Buffer Solution	Manufacture	Certified Value	Lot Number	Exp. date
Zero Oxygen Solution	Hanna	0.0 ± 0.1 @25°C	S0095/23	September 2028

Calibration Result

Inspection the accuracy of the Dissolved Oxygen (DO) Meter by using the following certificate reference material value.

Unit Under Calibration	CRM Standard DO	Actual value Reading	Error value Reading	Uncertainty of Measurement (\pm)
DO Electrode S/N KC1N53G5T	0.0 mg/L	0.00 mg/L	0.00 mg/L	N/A
	8.3 mg/L	8.26 mg/L	-0.04 mg/L	0.33 mg/L

The report uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

**** End of certificate ****

Certificate No. : HIT-2447-1923

Page : 1 of 2


CERTIFICATE OF CALIBRATION

Equipment :	COD Test Tube Heater		
Meter Model :	HI839150-02	Serial No. :	101450029111
Tube Heater :	25 Vial Capacity	Resolution :	0.1°C
Temperature Range :	(20 to 160)°C	Temperature of Reaction :	150°C
Manufacturer :	Hanna Instruments	Made in :	Romania
Condition As-Received :	New Product	Reference :	RE242195
Ambient Temperature :	(25 ± 2)°C	Relative Humidity :	(50 ± 15)% RH
Customer name :	Ecotech Water Systems Co., Ltd. 20 Soi Khaharomklao 74 Yaek 6, Ratphatthana, Saphansung, Bangkok 10240		
Received date :	11 November 2024		
Calibrate date :	19 November 2024		
Issue date :	20 November 2024		
Calibrated Location :	Hanna Instruments (Thailand) Ltd.		
Calibration Procedure :	This calibrator was conducted by using in-house: calibration procedure CP-04 by using certified reference standard instruments.		

Calibrated by :

☒ Mr. Pichit Petthong
☐ Mr. Channarong Soinak

Approved by :


Mr. Anan Suwanchaisakul

Authorized Signatory



This certificate was certified only for the instrument we calibrated.

This result of calibration was found accurate on date and place of calibration only.

** This certificate may not be reproduced other than in full, except with the prior written **
approval of the head of Hanna Instrument (Thailand).

Condition of this calibration result:

Reference Standard Instruments : This certification is traceable to the international unit of unit maintained through:

Instruments	Model	Serial No.	Certificate No.	Traceable
Data Acquisition Switch Unit	34970A	MY44065265	WK2407-141-1	WK Electric Co., Ltd.
Digital Thermo-Hygrometer	HT-771SD	AI.07155	24H41	Technology Promotion Association (Thailand-Japan).

Calibration Result:

Measurement Temperature Source Accuracy for COD Reactor.

Capacity (Vial)	Nominal Value (°C)	Average Value (°C)	Uncertainty of Measurement (±°C)
25 Vial	150.0	149.3	0.47

Unit : °C

(1A) 148.857	(2A) 149.223	(3A) 149.076	(4A) 149.256	(5A) 149.078
(1B) 148.934	(2B) 149.714	(3B) 150.210	(4B) 150.231	(5B) 149.181
(1C) 149.281	(2C) 149.807	(3C) 150.206	(4C) 149.128	(5C) 149.014
(1D) 149.039	(2D) 149.425	(3D) 148.788	(4D) 149.381	(5D) 148.605
(1E) 149.390	(2E) 149.200	(3E) 149.560	(4E) 148.930	(5E) 149.008

Figure: Shows the location of the temperature source.

The report uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

**** End of certificate ****

Certificate of Calibration

Certificate No. : 67-410114-3

Page : 1 of 2

Submitted by : Ecotech Water Co., Ltd.

20 Soi Kheharomklao 74 yaek 6, Ratphatthana, Saphansung, Bangkok 10240

Equipment : Digital Thermo-Hygrometer

Manufacturer : N/A

Model : HTC-2

Range Temperature : N/A °C

Resolution : 0.1 °C

Range Humidity : N/A %R.H.

Resolution : 1 %R.H.

Serial No. : N/A

ID No. : 66-410106-3

Environment : Ambient Temperature : $(23 \pm 2) ^\circ\text{C}$

Relative Humidity : $(50 \pm 15) \%$

Date of Received : 28 September 2024

Date of Calibration : 30 September 2024 to 02 October 2024

Date of Issue : 02 October 2024

Calibrated by : Chortip Samchusri

Calibration Method : This instrument was calibrated by In-house method comparison technique CAL-M4013 by compared with standard probe sensor humidity/temperature into humidity/temperature chamber.

Reference Standard Instruments : This certification is traceable to the International System of Units

Digital Indicator with Standard Probe Temp&Hum

ID No.	Cert. No.	Due Date	Traceability
400034 & 400035	SG-H-00611/67	04 Jan 2025	Success Gateway Co., Ltd., Accredited by TISI Calibration No.0268

Approved by :



(Permpon Chanpu)

Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 67-410114-3

Page : 2 of 2

UUC Condition As-Received : Good

Result of Calibration : Without Adjustment

Function : Temperature measurement (Mode : In)

Reference Humidity @ 50 %R.H.

Standard Temperature (°C)	UUC Reading (°C)	Correction (°C)	Uncertainty (± °C)
19.97	20.7	-0.7	0.46
25.03	25.6	-0.6	0.46
30.02	30.3	-0.3	0.46

Result of Calibration : Without Adjustment

Function : Humidity measurement

Reference Temperature @ 25 °C

Standard Humidity (%R.H.)	UUC Reading (%R.H.)	Correction (%R.H.)	Uncertainty (± %R.H.)
39.98	40	0	2.2
50.00	47	3	2.2
60.01	53	7	2.3

Remark

UUC : Unit Under Calibration

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

- o0o -

(Signature)



Certificate of Calibration

Certificate No. : 67-410114-2

Page : 1 of 2

Submitted by : Ecotech Water Co., Ltd.
20 Soi Kheharomklao 74 yaek 6, Ratphatthana, Saphansung, Bangkok 10240

Equipment : Digital Thermo-Hygrometer
Manufacturer : Digicon Model : TH-03A
Range Temperature : -10 °C to 50 °C Resolution : 0.1 °C
Range Humidity : 20 %R.H. to 99 %R.H. Resolution : 1 %R.H.
Serial No. : 365051554 ID No. : N/A

Environment : Ambient Temperature : $(23 \pm 2) ^\circ\text{C}$
Relative Humidity : $(50 \pm 15) \%$

Date of Received : 28 September 2024

Date of Calibration : 30 September 2024 to 02 October 2024

Date of Issue : 02 October 2024

Calibrated by : Chortip Samchusri

Calibration Method : This instrument was calibrated by In-house method comparison technique CAL-M4013
by compared with standard probe sensor humidity/temperature into humidity/temperature chamber.

Reference Standard Instruments : This certification is traceable to the International System of Units

Digital Indicator with Standard Probe Temp&Hum

ID No.	Cert. No.	Due Date	Traceability
400034 & 400035	SG-H-00611/67	04 Jan 2025	Success Gateway Co., Ltd., Accredited by TISI Calibration No.0268

Approved by :



(Permpon Chanpu)

Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 67-410114-2

Page : 2 of 2

UUC Condition As-Received : Good

Result of Calibration : Without Adjustment

Function : Temperature measurement (Mode : In)

Reference Humidity @ 50 %R.H.

Standard Temperature (°C)	UUC Reading (°C)	Correction (°C)	Uncertainty (± °C)
20.00	20.1	-0.1	0.46
25.02	25.1	-0.1	0.46
29.98	29.7	0.3	0.46

Result of Calibration : Without Adjustment

Function : Humidity measurement

Reference Temperature @ 25 °C

Standard Humidity (%R.H.)	UUC Reading (%R.H.)	Correction (%R.H.)	Uncertainty (± %R.H)
40.01	37	3	4.1
50.03	47	3	4.1
59.97	57	3	4.1

Remark

UUC : Unit Under Calibration

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

- o0o -

(Signature)



Certificate of Calibration

Certificate No. : 67-410114-1

Page : 1 of 2

Submitted by : Ecotech Water Co., Ltd.

20 Soi Kheharomklao 74 yaek 6, Ratphatthana, Saphansung, Bangkok 10240

Equipment : Digital Thermo-Hygrometer

Manufacturer : Digicon

Model : TH-03A

Range Temperature : -10 °C to 50 °C

Resolution : 0.1 °C

Range Humidity : 20 %R.H. to 99 %R.H.

Resolution : 1 %R.H.

Serial No. : 365052106

ID No. : N/A

Environment : Ambient Temperature : (23 ± 2) °C

Relative Humidity : (50 ± 15) %

Date of Received : 28 September 2024

Date of Calibration : 30 September 2024 to 02 October 2024

Date of Issue : 02 October 2024

Calibrated by : Chortip Samchusri

Calibration Method : This instrument was calibrated by In-house method comparison technique CAL-M4013 by compared with standard probe sensor humidity/temperature into humidity/temperature chamber.

Reference Standard Instruments : This certification is traceable to the International System of Units

Digital Indicator with Standard Probe Temp&Hum

ID No.

Cert. No.

Due Date

Traceability

400034 & 400035

SG-H-00611/67

04 Jan 2025

Success Gateway Co., Ltd., Accredited by TISI Calibration No.0268

Approved by :



(Permpon Chanpu)

Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



www.calibratech.co.th

Certificate of Calibration

Certificate No. : 67-410114-1

Page : 2 of 2

UUC Condition As-Received : Good

Result of Calibration : Temperature measurement (Mode : In)

Function : Temperature measurement

Reference Humidity @ 50 %R.H.

Standard Temperature (°C)	UUC Reading (°C)	Correction (°C)	Uncertainty (± °C)
19.98	20.3	-0.3	0.46
25.00	25.3	-0.3	0.46
30.01	29.9	0.1	0.46

Result of Calibration : Without Adjustment

Function : Humidity measurement

Reference Temperature @ 25 °C

Standard Humidity (%R.H.)	UUC Reading (%R.H.)	Correction (%R.H.)	Uncertainty (± %R.H)
40.05	38	2	3.1
50.02	48	2	3.1
60.02	58	2	3.2

Remark

UUC : Unit Under Calibration

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

- o0o -

P



Certificate of Calibration

Certificate No. : 67-200346-1

Page : 1 of 2

Submitted by : Ecotech Water Systems Co., Ltd.
20 Soi Kheharomklao 74 Yak 6, Ratphatthana, Saphansung, Bangkok 10240

Equipment : Electronic Balance
Manufacturer : OHAUS Model : PA214
Serial No. : 8328380168 ID No. : INS013
Capacity : 210 g Resolution : 0.0001 g

Environment : On site calibration was carried out at the Laboratory, Ecotech Water Systems Co., Ltd.
Ambient Temperature : (27.7 to 28.4) °C
Relative Humidity : (48.1 to 48.9) %
Air Pressure : 1009.0 mbar

Date of Received : 28 September 2024

Date of Calibration : 28 September 2024

Date of Issue : 30 September 2024

Calibrated by : Akaradath Thippichai

Calibration Method : In-house method CAL-M2001 based on UKAS Publication ref : LAB 14
Edition 7 - November 2022

Reference Standard Instruments : This certification is traceable to the International System of Units

Standard Weights

ID No.	Cert. No.	Due Date	Traceability
E261-E2624	C02232088	08 Nov 2024	National Institute of Metrology (Thailand), (NIMT)

Approved by :



(Satja Sangkhum)

Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 67-200346-1

Page : 2 of 2

Result of Calibration : After Adjustment

UUC Condition As-Received : Good

Departure of indication from nominal value


Nominal Value (g)	Correction (g)	Uncertainty \pm (g)	Error before Adjustment (g)
0.01	0.0000	0.00012	0.0000
0.1	0.0000	0.00012	0.0000
1	-0.0001	0.00013	0.0000
5	-0.0001	0.00013	0.0000
10	0.0000	0.00013	0.0000
20	-0.0001	0.00014	0.0002
50	0.0001	0.00015	0.0007
100	0.0001	0.00020	0.0014
150	0.0001	0.00038	0.0018
200	0.0002	0.00038	0.0026

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2.06$, providing a level of confidence of approximately 95%

Eccentric error

Load test : 50 g
 A B C D E
 0.0002 0.0001 -0.0002 0.0000 0.0000 g



Repeatability

Load test : 200 g
 Stdev. : 0.00005 g

- o0o -



Certificate of Calibration

Certificate No. : 67-400561-6

Page : 1 of 2

Submitted by : Ecotech Water Co., Ltd.

20 Soi Kheharomklao 74 Yaek 6, Ratphatthana, Saphansung, Bangkok 10240

Equipment : Temperature controlled enclosure (Incubator)

Manufacturer : Biobase

Model : BJPX-B400II

Range : N/A °C

Resolution : 0.1 °C

Serial No. : KYP400II2010002

ID No. : N/A

Environment : On site calibration was carried out at the Laboratory, Ecotech Water Co., Ltd.

Ambient Temperature : (25.3 to 25.8) °C

Relative Humidity : (44 to 48) %

Line Voltage : (225.0 to 226.5) V

Date of Received : 28 September 2024

Date of Calibration : 28 September 2024

Date of Issue : 02 October 2024

Calibrated by : Permpon Chanpu

Calibration Method : CAL-M4004, TLAS G-20

The temperature scale used was based on ITS-90

Reference Standard Instruments : This certification is traceable to the International System of Units
Standard Digital Thermometer with RTD Probe

<u>ID No.</u>	<u>Cert. No.</u>	<u>Due Date</u>	<u>Traceability</u>
400029 & 400043	67-400245-1	27 Oct 2024	National Institute of Metrology Thailand (NIMT)

Approved by :



(Permpon Chanpu)

Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 67-400561-6


Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Function : Temperature measurement

This instrument was setting air ventilation at position 0 (close)

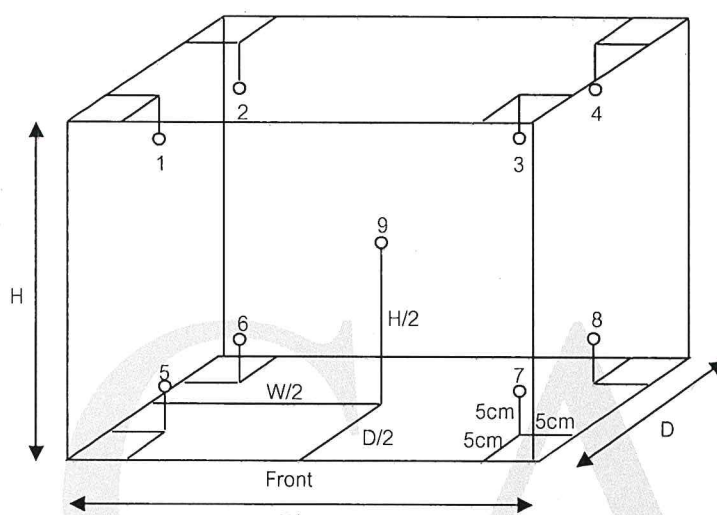

Inside of Chamber

W = 0.58 m

D = 0.55 m

H = 1.28 m

Capacity = 0.41 m³

Test Point (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Temperature (°C) @ Sensor No.									Uncertainty (± °C)
			1	2	3	4	5	6	7	8	9	
20.0	20.0	20.0	20.30	20.21	20.37	20.21	20.16	20.19	20.15	20.05	20.15	1.2

Test Point (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Uniformity (°C)	Measured Stability (°C)	Overall Variation (°C)
20.0	20.0	20.0	0.57	0.66	1.36

Remark The uncertainty is not combine uniformity of the air chamber

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

- o0o -

[Handwritten signature]



Certificate of Calibration

Certificate No. : 67-400561-5

Page : 1 of 2

Submitted by : Ecotech Water Co., Ltd.

20 Soi Kheharomklao 74 Yaek 6, Ratphatthana, Saphansung, Bangkok 10240

Equipment : Temperature controlled enclosure (Incubator)

Manufacturer : Biobase

Model : BJPX-B400II

Range : N/A °C

Resolution : 0.1 °C

Serial No. : KYP400II2310015

ID No. : N/A

Environment : On site calibration was carried out at the Laboratory, Ecotech Water Co., Ltd.

Ambient Temperature : (25.3 to 25.8) °C

Relative Humidity : (44 to 48) %

Line Voltage : (225.0 to 226.5) V

Date of Received : 28 September 2024

Date of Calibration : 28 September 2024

Date of Issue : 02 October 2024

Calibrated by : Permpon Chanpu

Calibration Method : CAL-M4004, TLAS G-20

The temperature scale used was based on ITS-90

Reference Standard Instruments : This certification is traceable to the International System of Units
Standard Digital Thermometer with RTD Probe

ID No.	Cert. No.	Due Date	Traceability
400029 & 400048	67-400444-1	02 Feb 2025	National Institute of Metrology Thailand (NIMT)

Approved by :



(Permpon Chanpu)

Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 67-400561-5


Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Function : Temperature measurement

This instrument was setting air ventilation at position 0 (close)

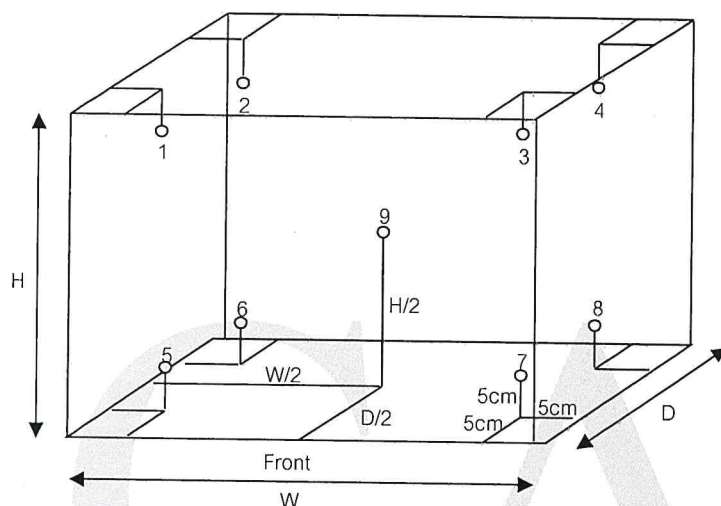

Inside of Chamber

W = 0.58 m

D = 0.55 m

H = 1.28 m

Capacity = 0.41 m³

Test Point (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Temperature (°C) @ Sensor No.									Uncertainty (± °C)
			1	2	3	4	5	6	7	8	9	
20.0	20.0	20.0	19.93	19.95	20.00	20.10	20.04	19.95	20.07	20.07	20.02	0.93

Test Point (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Uniformity (°C)	Measured Stability (°C)	Overall Variation (°C)
20.0	20.0	20.0	0.39	0.52	1.15

Remark The uncertainty is not combine uniformity of the air chamber

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

- oOo -

Handwritten signature



Certificate of Calibration

Certificate No. : 67-400561-2

Page : 1 of 2

Submitted by : Ecotech Water Co., Ltd.

20 Soi Kheharomklao 74 Yaek 6, Ratphatthana, Saphansung, Bangkok 10240

Equipment : Temperature controlled enclosure (Oven)

Manufacturer : Labtech

Model : LDO-080F

Range : N/A °C

Resolution : 0.1 °C

Serial No. : 081029024

ID No. : INS007

Environment : On site calibration was carried out at the Laboratory, Ecotech Water Co., Ltd.

Ambient Temperature : (26.0 to 27.0) °C

Relative Humidity : (52 to 56) %

Line Voltage : (225.5 to 228.5) V

Date of Received : 28 September 2024

Date of Calibration : 28 September 2024

Date of Issue : 02 October 2024

Calibrated by : Permpon Chanpu

Calibration Method : CAL-M4004, TLAS G-20

The temperature scale used was based on ITS-90

Reference Standard Instruments : This certification is traceable to the International System of Units

Standard Digital Thermometer with Thermocouple probe

ID No.

Cert. No.

Due Date

Traceability

400046 & 400023 67-400198-1

01 Oct 2024

National Institute of Metrology Thailand (NIMT)

Approved by :



(Permpon Chanpu)

Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 67-400561-2


Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Function : Temperature measurement

This instrument was setting air ventilation at position 0 (close)

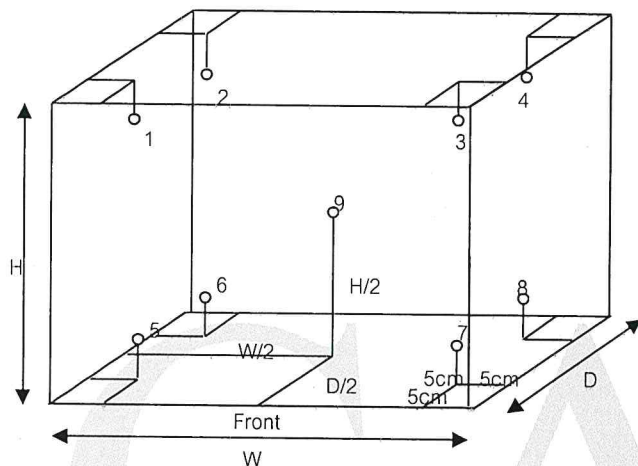

Inside of Chamber

W = 0.50 m

D = 0.40 m

H = 0.40 m

Capacity = 0.08 m³

Test Point (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Temperature (°C) @ Sensor No.									Uncertainty (± °C)
			1	2	3	4	5	6	7	8	9	
104.0	104.0	104.0	104.0	103.1	103.9	103.8	103.0	103.0	103.3	103.7	104.2	1.4
180.0	180.0	180.0	178.9	179.0	178.8	179.3	178.0	177.8	178.4	179.1	180.0	2.9

Test Point (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Uniformity (°C)	Measured Stability (°C)	Overall Variation (°C)
104.0	104.0	104.0	1.5	1.1	3.1
180.0	180.0	180.0	3.2	2.3	6.1

Remark The uncertainty is not combine uniformity of the air chamber

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k = 2 , providing a level of confidence of approximately 95%

- o0o -

Handwritten signature or mark.



Certificate of Calibration

Certificate No. : 67-420113-2

Page : 1 of 2

Submitted by : Ecotech Water Co., Ltd.
20 Soi Kheharomklao 74 yaek 6, Ratphatthana, Saphansung, Bangkok 10240

Equipment : pH Meter with electrode
pH meter
Manufacturer : Eutech Model : PC 450
Range : N/A pH Resolution : 0.01 pH
Serial No. : 2535550 ID No. : N/A
Electrode
Model : ECFC7252201B Serial No. : 01X099323 172

Environment : On site calibration was carried out at the Laboratory, Ecotech Water Co., Ltd.
Ambient Temperature : (25.5 to 26.0)° C
Relative Humidity : (50 to 55) %

Date of Received : 28 September 2024

Date of Calibration : 28 September 2024

Date of Issue : 02 October 2024

Calibrated by : Permpon Chanpu

Calibration Method : In-house method CAL-M4201 direct measurement by using standard voltage calibrator and using certified reference material (CRM)

Reference Standard Instruments : This certification is traceable to the International System of Units

1. Multiproduct Calibrator

ID No.	Cert. No.	Due Date	Traceability
400005	SG-E-00307/66	23 Aug 2025	National Institute of Metrology Thailand (NIMT)

2. Standard Buffer Solution

pH	Cert. No.	Lot No.	Exp. Date	Traceability
4.008	61293328	1027612	15 Sep 2026	CPA Chem Ltd. Accredited to ISO 17034 and ISO/IEC 17025
6.987	61297593	1027614	15 Sep 2025	CPA Chem Ltd. Accredited to ISO 17034 and ISO/IEC 17025
10.010	61306165	1027613	15 Sep 2025	CPA Chem Ltd. Accredited to ISO 17034 and ISO/IEC 17025

Approved by :



(Permpon Chanpu)

Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 67-420113-2

Page : 2 of 2

Result of Calibration :

UUC Condition As-Received : Good

Function : Electrical measurement

pH meter

Performing standard curve by Multiproduct Calibrator at pH (4,7,10)

Adjustment Curve at nominal pH	Applied Voltage (mV)	Nominal Value (pH)	UUC Reading		Correction (mV)	Uncertainty (± mV)
			(pH)	(mV)		
4, 7, 10	177.4800	4	4.00	177.6	-0.1	0.12
	0.0000	7	7.00	0.1	-0.1	0.086
	-177.4800	10	10.00	-177.5	0.0	0.12

Function : pH meter with electrode

Performing a three - buffer standard curve using buffer nominal pH (4,7,10)

Adjustment Curve at nominal pH	Standard Buffer (pH)	UUC Reading (pH)	Correction (pH)	Uncertainty (± pH)
4, 7, 10	4.008	4.01	0.00	0.0097
	6.987	7.00	-0.01	0.011
	10.010	10.01	0.00	0.014

Remark

UUC : Unit Under Calibration

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurment was based on a standard uncertainty multiplied by a coverage factor $k = 2$,
providing a level of confidence of approximately 95%

- o0o -

[Handwritten signature]



Certificate of Calibration

Certificate No. : 67-400562-2

Page : 1 of 2

Submitted by : Ecotech Water Co., Ltd.
20 Soi Kheharomklao 74 yaek 6, Ratphatthana, Saphansung, Bangkok 10240

Equipment : Temperature Indicator with Thermistor Probe
Temperature Indicator

Manufacturer :	Eutech	Model :	PC 450
Range :	N/A °C	Resolution :	0.1 °C
Serial No. :	2535550	ID No. :	N/A
Thermistor probe			
Model :	N/A	Sheath Material :	Stainless
Diameter :	3.5 mm.	Length :	100 mm.
Serial No. :	CONSEN91W 141	ID No. :	N/A

Environment : On site calibration was carried out at the Laboratory, Ecotech Water Co., Ltd.

Ambient Temperature :	(25.5 to 26.0) °C
Relative Humidity :	(50 to 55) %
Line Voltage :	(225.0 to 225.9) VAC

Date of Received : 28 September 2024

Date of Calibration : 28 September 2024

Date of Issue : 02 October 2024

Calibrated by : Permpon Chanpu

Calibration Method : This instrument was calibrated by In-house method comparison technique CAL-M4003 by compared with PRT in the liquid bath at the constant controlled temperature.

The temperature scale used was based on ITS-90

Reference Standard Instruments : This certification is traceable to the International System of Units

1. Platinum Resistance Thermometer (PRT)

ID No.	Cert. No.	Due Date	Traceability
400002	TT-0095-24	01 Jul 2026	National Institute of Metrology Thailand (NIMT)

2. Standard Digital Thermometer

ID No.	Cert. No.	Due Date	Traceability
400033	24E633	21 Feb 2026	National Institute of Metrology Thailand (NIMT)

Approved by :



(Permpon Chanpu)

Supervisor



Certificate of Calibration

Certificate No. : 67-400562-2

Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Function : Temperature measurement

Immersion Depth (mm.)	Standard Reading (° C)	UUC Reading (° C)	Correction (° C)	Uncertainty (± ° C)
100	20.004	20.1	-0.1	0.19
100	25.003	25.0	0.0	0.19
100	30.002	30.0	0.0	0.19

Remark

UUC : Unit Under Calibration

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

- ๐0๐ -

7



Certificate of Calibration

Certificate No. : 67-420113-1

Page : 1 of 2

Submitted by : Ecotech Water Co., Ltd.

20 Soi Kheharomklao 74 yaek 6, Ratphatthana, Saphansung, Bangkok 10240

Equipment : pH Meter with electrode

pH meter

Manufacturer : Eutech

Model : PC 700

Range : N/A

pH

Resolution : 0.01 pH

Serial No. : 2728583

ID No. : N/A

Electrode

Model : ECFC7252201B

Serial No. : 1062322022

Environment : On site calibration was carried out at the Laboratory, Ecotech Water Co., Ltd.

Ambient Temperature : (25.5 to 26.0)° C

Relative Humidity : (50 to 55) %

Date of Received : 28 September 2024

Date of Calibration : 28 September 2024

Date of Issue : 02 October 2024

Calibrated by : Permpon Chanpu

Calibration Method : In-house method CAL-M4201 direct measurement by using standard voltage calibrator and using certified reference material (CRM)

Reference Standard Instruments : This certification is traceable to the International System of Units

1. Multiproduct Calibrator

ID No.	Cert. No.	Due Date	Traceability
400005	SG-E-00307/66	23 Aug 2025	National Institute of Metrology Thailand (NIMT)

2. Standard Buffer Solution

pH	Cert. No.	Lot No.	Exp. Date	Traceability
4.008	61293328	1027612	15 Sep 2026	CPA Chem Ltd. Accredited to ISO 17034 and ISO/IEC 17025
6.987	61297593	1027614	15 Sep 2025	CPA Chem Ltd. Accredited to ISO 17034 and ISO/IEC 17025
10.010	61306165	1027613	15 Sep 2025	CPA Chem Ltd. Accredited to ISO 17034 and ISO/IEC 17025

Approved by :



(Permpon Chanpu)

Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 67-420113-1

Page : 2 of 2

Result of Calibration :

UUC Condition As-Received : Good

Function : Electrical measurement

pH meter

Performing standard curve by Multiproduct Calibrator at pH (4,7,10)

Adjustment Curve at nominal pH	Applied Voltage (mV)	Nominal Value (pH)	UUC Reading		Correction (mV)	Uncertainty (± mV)
			(pH)	(mV)		
4, 7, 10	177.4800	4	4.00	175.1	2.4	0.12
	0.0000	7	7.00	0.0	0.0	0.086
	-177.4800	10	10.00	-175.1	-2.4	0.12

Function : pH meter with electrode

Performing a three - buffer standard curve using buffer nominal pH (4,7,10)

Adjustment Curve at nominal pH	Standard Buffer (pH)	UUC Reading (pH)	Correction (pH)	Uncertainty (± pH)
4, 7, 10	4.008	4.01	0.00	0.0097
	6.987	7.00	-0.01	0.011
	10.010	10.01	0.00	0.014

Remark

UUC : Unit Under Calibration

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurment was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

- 000 -

[Signature]



Certificate of Calibration

Certificate No. : 67-430047-1

Page : 1 of 2

Submitted by : Ecotech Water Co., Ltd.

20 Soi Kheharomklao 74 yaek 6, Ratphatthana, Saphansung, Bangkok 10240

Equipment : Digital Conductivity meter with probe

Manufacturer : Eutech Model : PC 700

Serial No. : 2728583 ID No. : N/A

Electrode

Model : N/A Serial No. : CONSEN9501D 102

Environment : On site calibration was carried out at the Laboratory, Ecotech Water Co., Ltd.

Ambient Temperature (25.5 to 26.0) °C

Relative Humidity (50 to 55) %

Date of Received : 28 September 2024

Date of Calibration : 28 September 2024

Date of Issue : 02 October 2024

Calibrated by : Permpon Chanpu

Calibration Method : In-house method CAL-M4301 direct measurement by conductivity buffer solution

Reference Standard Instruments : This certification is traceable to the International System of Units

Standard Buffer Solution

<u>Material</u>	<u>Lot No.</u>	<u>Exp. Date</u>	<u>Traceability</u>
84 µS/cm	7824	16 June 2025	National Institute of Standards and Technology (NIST), U.S.A., S.R.M.
1413 µS/cm	970986	25 April 2025	CPA Chem Ltd. Accredited to ISO 17034 and ISO/IEC 17025
12.88 mS/cm	970987	25 April 2025	CPA Chem Ltd. Accredited to ISO 17034 and ISO/IEC 17025

Approved by :



(Permpon Chanpu)

Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 67-430047-1

Page : 2 of 2

Result of Calibration :

UUC Condition As-Received : Good

Function : Conductivity measurement

Before Adjustment

Standard Conductivity Solution	UUC Reading	Correction	Uncertainty (±)	Unit
84*	94.2	-10.2	1.1	μS/cm
1413	1284	129	9.0	μS/cm
12.88	12.31	0.57	0.082	mS/cm

After Adjustment : at 84, 1413 μS/cm 12.880 mS/cm

Standard Conductivity Solution	UUC Reading	Correction	Uncertainty (±)	Unit
84*	84.0	0.0	1.1	μS/cm
1413	1413	0	9.0	μS/cm
12.88	12.88	0.00	0.082	mS/cm

Remark

UUC : Unit Under Calibration

* This parameter are out of accreditation's scope.

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$,
providing a level of confidence of approximately 95%

- ๐0๐ -

7



Certificate of Calibration

Certificate No. : 67-400562-1

Page : 1 of 2

Submitted by : Ecotech Water Co., Ltd.
20 Soi Kheharomklao 74 yaek 6, Ratphatthana, Saphansung, Bangkok 10240

Equipment : Temperature Indicator with Thermistor Probe
Temperature Indicator

Manufacturer : Eutech Model : PC 700
Range : N/A °C Resolution : 0.1 °C
Serial No. : 2728583 ID No. : N/A

Thermistor probe

Model : N/A Sheath Material : Stainless
Diameter : 3.5 mm. Length : 100 mm.
Serial No. : CONSEN9501D 102 ID No. : N/A

Environment : On site calibration was carried out at the Laboratory, Ecotech Water Co., Ltd.

Ambient Temperature : (25.5 to 26.0) °C
Relative Humidity : (50 to 55) %
Line Voltage : (225.0 to 225.9) VAC

Date of Received : 28 September 2024

Date of Calibration : 28 September 2024

Date of Issue : 02 October 2024

Calibrated by : Permpon Chanpu

Calibration Method : This instrument was calibrated by In-house method comparison technique CAL-M4003 by compared with PRT in the liquid bath at the constant controlled temperature.

The temperature scale used was based on ITS-90

Reference Standard Instruments : This certification is traceable to the International System of Units

1. Platinum Resistance Thermometer (PRT)

ID No.	Cert. No.	Due Date	Traceability
400002	TT-0095-24	01 Jul 2026	National Institute of Metrology Thailand (NIMT)

2. Standard Digital Thermometer

ID No.	Cert. No.	Due Date	Traceability
400033	24E633	21 Feb 2026	National Institute of Metrology Thailand (NIMT)

Approved by :



(Permpon Chanpu)

Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 67-400562-1

Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Function : Temperature measurement

Immersion Depth (mm.)	Standard Reading (° C)	UUC Reading (° C)	Correction (° C)	Uncertainty (± ° C)
100	20.006	20.2	-0.2	0.19
100	25.005	25.1	-0.1	0.19
100	30.003	30.0	0.0	0.19

Remark

UUC : Unit Under Calibration

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

- ๐0๐ -

[Handwritten Signature]



Certificate of Calibration

Certificate No. : 67-400562-3

Page : 1 of 2

Submitted by : Ecotech Water Co., Ltd.
20 Soi Kheharomklao 74 yaek 6, Ratphatthana, Saphansung, Bangkok 10240

Equipment : Temperature Indicator with Thermistor Probe
Temperature Indicator

Manufacturer :	Eutech	Model :	PC 700
Range :	N/A °C	Resolution :	0.1 °C
Serial No. :	3082600	ID No. :	N/A
Thermistor probe			
Model :	N/A	Sheath Material :	Stainless
Diameter :	3.5 mm.	Length :	100 mm.
Serial No. :	CONSEN9501D 028	ID No. :	N/A

Environment : On site calibration was carried out at the Laboratory, Ecotech Water Co., Ltd.

Ambient Temperature :	(25.5 to 26.0) °C
Relative Humidity :	(50 to 55) %
Line Voltage :	(225.0 to 225.9) VAC

Date of Received : 28 September 2024

Date of Calibration : 28 September 2024

Date of Issue : 02 October 2024

Calibrated by : Permpon Chanpu

Calibration Method : This instrument was calibrated by In-house method comparison technique CAL-M4003 by compared with PRT in the liquid bath at the constant controlled temperature.

The temperature scale used was based on ITS-90

Reference Standard Instruments : This certification is traceable to the International System of Units

1. Platinum Resistance Thermometer (PRT)

<u>ID No.</u>	<u>Cert. No.</u>	<u>Due Date</u>	<u>Traceability</u>
400002	TT-0095-24	01 Jul 2026	National Institute of Metrology Thailand (NIMT)

2. Standard Digital Thermometer

<u>ID No.</u>	<u>Cert. No.</u>	<u>Due Date</u>	<u>Traceability</u>
400033	24E633	21 Feb 2026	National Institute of Metrology Thailand (NIMT)

Approved by :



(Permpon Chanpu)

Supervisor



Certificate of Calibration

Certificate No. : 67-400562-3

Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Function : Temperature measurement

Immersion Depth (mm.)	Standard Reading (° C)	UUC Reading (° C)	Correction (° C)	Uncertainty (± ° C)
100	20.003	20.4	-0.4	0.19
100	25.005	25.3	-0.3	0.19
100	30.002	30.2	-0.2	0.19

Remark

UUC : Unit Under Calibration

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

- 000 -

2



Certificate of Calibration

Certificate No. : 67-420113-3

Page : 1 of 2

Submitted by : Ecotech Water Co., Ltd.

20 Soi Kheharomklao 74 yaek 6, Ratphatthana, Saphansung, Bangkok 10240

Equipment : pH Meter with electrode

pH meter

Manufacturer : Eutech

Model : PC 700

Range : N/A pH

Resolution : 0.01 pH

Serial No. : 3082600

ID No. : N/A

Electrode

Model : ECFC7252201B

Serial No. : 13042322006

Environment : On site calibration was carried out at the Laboratory, Ecotech Water Co., Ltd.

Ambient Temperature : (25.5 to 26.0)° C

Relative Humidity : (50 to 55) %

Date of Received : 28 September 2024

Date of Calibration : 28 September 2024

Date of Issue : 02 October 2024

Calibrated by : Permpon Chanpu

Calibration Method : In-house method CAL-M4201 direct measurement by using standard voltage calibrator and using certified reference material (CRM)

Reference Standard Instruments : This certification is traceable to the International System of Units

1. Multiproduct Calibrator

ID No.	Cert. No.	Due Date	Traceability
400005	SG-E-00307/66	23 Aug 2025	National Institute of Metrology Thailand (NIMT)

2. Standard Buffer Solution

pH	Cert. No.	Lot No.	Exp. Date	Traceability
4.008	61293328	1027612	15 Sep 2026	CPA Chem Ltd. Accredited to ISO 17034 and ISO/IEC 17025
6.987	61297593	1027614	15 Sep 2025	CPA Chem Ltd. Accredited to ISO 17034 and ISO/IEC 17025
10.010	61306165	1027613	15 Sep 2025	CPA Chem Ltd. Accredited to ISO 17034 and ISO/IEC 17025

Approved by :

(Permpon Chanpu)

Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 67-420113-3

Page : 2 of 2

Result of Calibration :

UUC Condition As-Received : Good

Function : Electrical measurement

pH meter

Performing standard curve by Multiproduct Calibrator at pH (4,7,10)

Adjustment Curve at nominal pH	Applied Voltage (mV)	Nominal Value (pH)	UUC Reading		Correction (mV)	Uncertainty (± mV)
			(pH)	(mV)		
4, 7, 10	177.4800	4	4.00	177.4	0.1	0.12
	0.0000	7	7.00	0.1	-0.1	0.086
	-177.4800	10	10.00	-177.4	-0.1	0.12

Function : pH meter with electrode

Performing a three - buffer standard curve using buffer nominal pH (4,7,10)

Adjustment Curve at nominal pH	Standard Buffer (pH)	UUC Reading (pH)	Correction (pH)	Uncertainty (± pH)
4, 7, 10	4.008	4.01	0.00	0.0097
	6.987	7.00	-0.01	0.011
	10.010	10.01	0.00	0.014

Remark

UUC : Unit Under Calibration

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurment was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

- oOo -

Handwritten signature



Certificate of Calibration

Certificate No. : 67-430047-2

Page : 1 of 2

Submitted by : Ecotech Water Co., Ltd.

20 Soi Kheharomklao 74 yaek 6, Ratphatthana, Saphansung, Bangkok 10240

Equipment : Digital Conductivity meter with probe

Manufacturer : Eutech Model : PC 700

Serial No. : 3082600 ID No. : N/A

Electrode

Model : N/A Serial No. : CONSEN9501D 028

Environment : On site calibration was carried out at the Laboratory, Ecotech Water Co., Ltd.

Ambient Temperature (25.5 to 26.0) °C

Relative Humidity (50 to 55) %

Date of Received : 28 September 2024

Date of Calibration : 28 September 2024

Date of Issue : 02 October 2024

Calibrated by : Permpon Chanpu

Calibration Method : In-house method CAL-M4301 direct measurement by conductivity buffer solution

Reference Standard Instruments : This certification is traceable to the International System of Units

Standard Buffer Solution

<u>Material</u>	<u>Lot No.</u>	<u>Exp. Date</u>	<u>Traceability</u>
84 µS/cm	7824	16 June 2025	National Institute of Standards and Technology (NIST), U.S.A., S.R.M.
1413 µS/cm	970986	25 April 2025	CPA Chem Ltd. Accredited to ISO 17034 and ISO/IEC 17025
12.88 mS/cm	970987	25 April 2025	CPA Chem Ltd. Accredited to ISO 17034 and ISO/IEC 17025

Approved by :



(Permpon Chanpu)

Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 67-430047-2

Page : 2 of 2

Result of Calibration :

UUC Condition As-Received : Good

Function : Conductivity measurement

Before Adjustment

Standard Conductivity Solution	UUC Reading	Correction	Uncertainty (±)	Unit
84*	107.6	-23.6	1.1	μS/cm
1413	1094	319	9.0	μS/cm
12.88	12.98	-0.10	0.082	mS/cm

After Adjustment : at 84, 1413 μS/cm 12.880 mS/cm

Standard Conductivity Solution	UUC Reading	Correction	Uncertainty (±)	Unit
84*	84.0	0.0	1.1	μS/cm
1413	1413	0	9.0	μS/cm
12.88	12.88	0.00	0.082	mS/cm

Remark

UUC : Unit Under Calibration

* This parameter are out of accreditation's scope.

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

- ๐0๐ -



Certificate of Calibration

Certificate No. : 67-400561-1

Page : 1 of 2

Submitted by : Ecotech Water Co., Ltd.

20 Soi Kheharomklao 74 Yaek 6, Ratphatthana, Saphansung, Bangkok 10240

Equipment : Temperature controlled enclosure (Refrigerator)

Manufacturer : Every Digital

Model : N/A

Range : N/A °C

Resolution : 0.1 °C

Serial No. : ASS1001

ID No. : INS005

Environment : On site calibration was carried out at the Laboratory, Ecotech Water Co., Ltd.

Ambient Temperature : (25.5 to 26.0) °C

Relative Humidity : (50 to 55) %

Line Voltage : (225.0 to 226.5) V

Date of Received : 28 September 2024

Date of Calibration : 28 September 2024

Date of Issue : 02 October 2024

Calibrated by : Permpon Chanpu

Calibration Method : CAL-M4004, TLAS G-20

The temperature scale used was based on ITS-90

Reference Standard Instruments : This certification is traceable to the International System of Units
Standard Digital Thermometer with RTD Probe

ID No.	Cert. No.	Due Date	Traceability
400046 & 400047	67-400442-2	27 Jan 2025	National Institute of Metrology Thailand (NIMT)

Approved by :



(Permpon Chanpu)

Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 67-400561-1


Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Function : Temperature measurement

This instrument was setting air ventilation at position 0 (close)

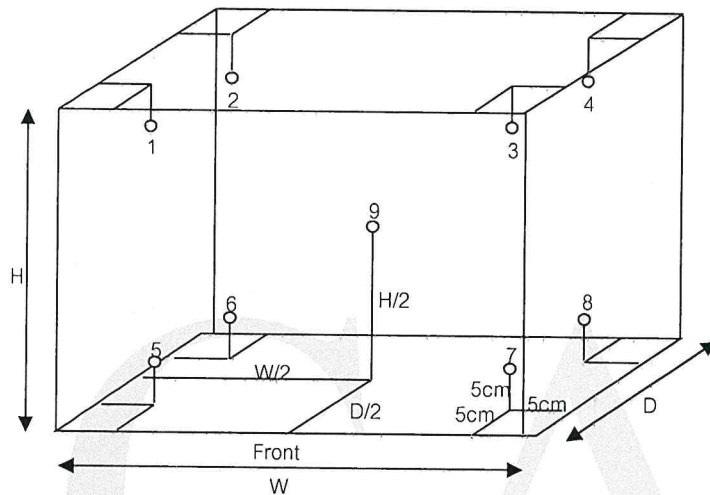

Inside of Chamber

W = 1.00 m

D = 0.50 m

H = 1.35 m

Capacity = 0.68 m³

Test Point (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Temperature (°C) @ Sensor No.									Uncertainty (± °C)
			1	2	3	4	5	6	7	8	9	
4.0	3.0	3.0	4.07	3.83	4.14	3.48	4.04	4.06	3.39	3.73	3.24	0.37

Test Point (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Uniformity (°C)	Measured Stability (°C)	Overall Variation (°C)
4.0	3.0	3.0	0.93	0.03	0.95

Remark The uncertainty is not combine uniformity of the air chamber

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

- o0o -

2



Certificate of Calibration

Certificate No. : 67-400561-4 **Page : 1 of 2**

Submitted by : Ecotech Water Co., Ltd.
20 Soi Kheharomklao 74 Yaek 6, Ratphatthana, Saphansung, Bangkok 10240

Equipment : Temperature controlled enclosure (Refrigerator)
Manufacturer : S-Cool **Model :** N/A
Range : N/A °C **Resolution :** 1 °C
Serial No. : Eco-Ins14 **ID No. :** N/A

Environment : On site calibration was carried out at the Laboratory, Ecotech Water Co., Ltd.
Ambient Temperature : (25.5 to 26.0) °C
Relative Humidity : (50 to 55) %
Line Voltage : (225.0 to 226.5) V

Date of Received : 28 September 2024

Date of Calibration : 28 September 2024

Date of Issue : 02 October 2024

Calibrated by : Permpon Chanpu

Calibration Method : CAL-M4004, TLAS G-20

The temperature scale used was based on ITS-90

Reference Standard Instruments : This certification is traceable to the International System of Units
Standard Digital Thermometer with RTD Probe

ID No.	Cert. No.	Due Date	Traceability
400046 & 400042	67-400442-1	26 Jan 2025	National Institute of Metrology Thailand (NIMT)

Approved by :



(Permpon Chanpu)

Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 67-400561-4


Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Function : Temperature measurement

This instrument was setting air ventilation at position 0 (close)

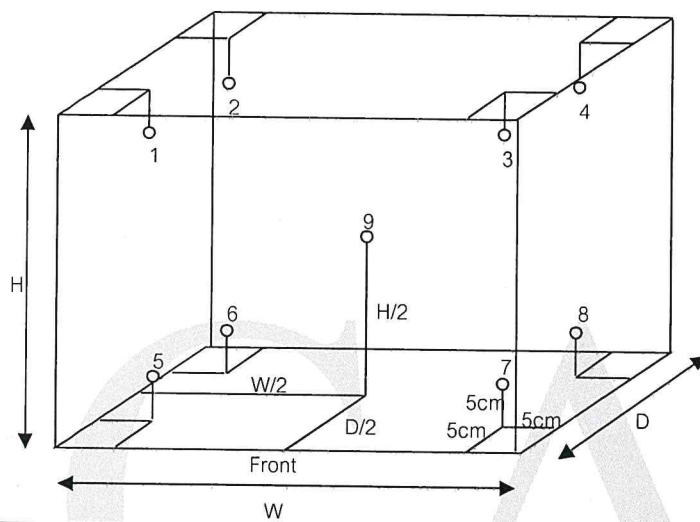

Inside of Chamber

W = 1.02 m

D = 0.44 m

H = 1.30 m

Capacity = 0.58 m³

Test Point (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Temperature (°C) @ Sensor No.									Uncertainty (± °C)
			1	2	3	4	5	6	7	8	9	
4.0	3.0	3.0	5.60	4.97	4.63	4.38	4.94	4.81	4.01	3.89	4.07	1.1

Test Point (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Uniformity (°C)	Measured Stability (°C)	Overall Variation (°C)
4.0	3.0	3.0	1.94	0.44	2.33

Remark The uncertainty is not combine uniformity of the air chamber

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

- o0o -

7





Bangkok High Lab Co.,Ltd.

4/176 Soi Ladplakao 66, Ladplakao Rd., Anusawari, Bangkhen, Bangkok 10220

Tel: (662) 971-5800

Fax: (662) 971-5300

Website: www.bangkokhighlab.com

E-mail: info@bangkokhighlab.com



NSC-TISI-TIS 17025

CALIBRATION 0366

CERTIFICATE OF CALIBRATION

Certificate No : S2024/091

Page : 1/5

Order No : 122/2024

Customer : Ecotech Water Systems Co.,Ltd
Address : 20 Kheha Rom Klao 74 Yeak 6, Ratphatthana, Saphansung, Bangkok 10240
Instrument : UV/VIS spectrophotometer
Manufacture : Rayleigh
Model : VIS-723G
Serial Number : 00080889
Environment : Temperature (25.2 - 25.2)° C
: Humidity (52 - 51) %RH
Received Date : May 23, 2024
Calibration Date : May 23, 2024
Issued Date : May 24, 2024
Calibrate Status : No Adjustment
Calibration Area : Customer area
Roomname : Laboratory Room of Ecotech Water Systems Co.,Ltd

Calibrated By : Pacharapol
(Mr. Pacharapol Kwanbang)
Calibration Engineer

Approved By : [Signature]
(Mr. Wanchai Meesiri)
Manager

This calibration certificate shall not be reproduced other than in full except with the prior written approval of the Bangkok High Lab Co.,Ltd.



Certificate No : S2024/091

Page : 2/5

1. Photometric Accuracy

CRMs: Neutral Density Glass Filters

CRMs Serial Number: 10563

Traceability: Traceable to NIST, U.S.A. through Neutral density filters NIST SRM 930e & 1930, Double Aperture method through Starna certificate report no.113594

Spectral slit width : 2.00 nm

1.1 Reading scale at 420.0 nm

Filter STDs (Abs) Certificate	Average Measured Value (A)	Correction (A)	Uncertainty ± (A)
0.0000	0.000	0.0000	0.0028
0.5604	0.557	0.0034	0.0044
1.0723	1.068	0.0043	0.0038
2.1753	2.170	0.0053	0.0064

1.2 Reading scale at 440.0 nm

Filter STDs (Abs) Certificate	Average Measured Value (A)	Correction (A)	Uncertainty ± (A)
0.0000	0.000	0.0000	0.0028
0.5503	0.547	0.0033	0.0040
1.0467	1.042	0.0047	0.0040
2.1117	2.107	0.0047	0.0064

1.3 Reading scale at 465.0 nm

Filter STDs (Abs) Certificate	Average Measured Value (A)	Correction (A)	Uncertainty ± (A)
0.0000	0.000	0.0000	0.0028
0.4996	0.496	0.0036	0.0034
0.9649	0.962	0.0029	0.0040
1.9646	1.960	0.0046	0.0060

1.4 Reading scale at 546.1 nm

Filter STDs (Abs) Certificate	Average Measured Value (A)	Correction (A)	Uncertainty ± (A)
0.0000	0.000	0.0000	0.0028
0.5136	0.515	-0.0014	0.0028
0.9765	0.975	0.0015	0.0028
1.9848	1.985	-0.0002	0.0064



Bangkok High Lab Co.,Ltd.

4/176 Soi Ladplakao 66, Ladplakao Rd., Anusawari, Bangkok, Bangkok 10220

Tel: (662) 971-5800

Fax: (662) 971-5300

Website: www.bangkokhighlab.com

E-mail: info@bangkokhighlab.com



NSC-TISI-TIS 17025
CALIBRATION 0366

Certificate No : S2024/091

Page : 3/5

1.5 Reading scale at 590.0 nm

Filter STDs (Abs) Certificate	Average Measured Value (A)	Correction (A)	Uncertainty ± (A)
0.0000	0.000	0.0000	0.0028
0.5424	0.539	0.0034	0.0029
1.0130	1.010	0.0030	0.0029
2.0238	2.022	0.0018	0.0061

1.6 Reading scale at 635.0 nm

Filter STDs (Abs) Certificate	Average Measured Value (A)	Correction (A)	Uncertainty ± (A)
0.0000	0.000	0.0000	0.0028
0.5265	0.523	0.0035	0.0030
0.9667	0.962	0.0047	0.0031
1.9145	1.909	0.0055	0.0062

2. Photometric Accuracy

CRMs: Potassium Dichromate in Perchloric acid

CRMs Serial Number: 132023

Blank Serial Number: 128038

Traceability: Traceable to NIST, U.S.A. through crystalline potassium dichromate NIST SRM 935a through Starna certificate report no.120920

Spectral slit width : 2.00 nm

Wavelength (nm)	Certificate (Abs)	Average Measured Value (A)	Correction (A)	Uncertainty ± (A)
235	0.0000	#N/A	#N/A	#N/A
	0.7351	#N/A	#N/A	#N/A
257	0.0000	#N/A	#N/A	#N/A
	0.8564	#N/A	#N/A	#N/A
313	0.0000	#N/A	#N/A	#N/A
	0.2855	#N/A	#N/A	#N/A
350	0.0000	#N/A	#N/A	#N/A
	0.6363	#N/A	#N/A	#N/A



Certificate No : S2024/091

Page : 4/5

3. Wavelength Accuracy

Spectral slit width : 2.00 nm

3.1 CRMs: Holmium Glass Filter

CRMs Serial Number: 10763

Traceability Traceable to NIST Holmium oxide filter NIST SRM 2034, through Starna certificate report no. 113607

Filter STDs (nm) Certificate	Average Measured Value (nm)	Correction (nm)	Uncertainty ± (nm)
241.74	#N/A	#N/A	#N/A
279.44	#N/A	#N/A	#N/A
287.98	#N/A	#N/A	#N/A
334.10	333.6	0.50	0.12
361.00	360.2	0.80	0.12
418.61	418.0	0.61	0.12
453.63	452.8	0.83	0.12
460.05	459.2	0.85	0.12
536.66	535.8	0.86	0.12
637.98	637.2	0.78	0.12

3.2 CRMs: Didymium Glass Filter

CRMs Serial Number: 10764

Traceability Traceable to NIST Didymium filter NIST SRM 2034, through Starna certificate report no. 113608

Filter STDs (nm) Certificate	Average Measured Value (nm)	Correction (nm)	Uncertainty ± (nm)
585.29	584.8	0.49	0.12
684.49	684.0	0.49	0.12
740.18	739.6	0.58	0.12
748.48	748.8	-0.32	0.12
807.03	806.6	0.43	0.12
879.27	878.6	0.67	0.12



Bangkok High Lab Co.,Ltd.
4/176 Soi Ladplakao 66, Ladplakao Rd., Anusawari, Bangkhen, Bangkok 10220
Tel: (662) 971-5800 Fax: (662) 971-5300
Website: www.bangkokhighlab.com E-mail: info@bangkokhighlab.com



Certificate No : S2024/091

Page : 5/5

4. *Stray Light

CRMs: Potassium Chloride aqueous solution

CRMs Serial Number: 14912

Blank Serial Number: 14958

Traceability Traceable to NIST, U.S.A. potassium chloride NIST SRM2032, through Starna certificate report no.113597

Spectral slit width : 2.00 nm

Wavelength (nm)	Certificate	Average Measured
201.13	>2A	#N/A
201.13	<1%T	#N/A

5. *Spectral Resolution

CRMs: Toluene in Hexane

CRMs Serial Number: 14812

Blank Serial Number: 14803

Traceability Traceable to toluene in hexane NIST SRM2034,through Starna certificate report no. 113598

Spectral slit width (nm)	Abs Ratio
0.5	#N/A
1.0	#N/A
1.5	#N/A
2.0	#N/A
3.0	#N/A

Note : * "Not TISI Accredited" in this certificate have been included for completeness

Remark: 1 Calibrate Method

- 1.1 Photometric and Wavelength accuracy: In-house method W-SER-001 based on ASTM E925-02 and ASTM E275-01
- 1.2 Stray light: Measuring the CRMs in both absorbance and transmittance unit at wavelength 201.23 nm. Base on European Pharmacopoeia V.6.19.3 1984
- 1.3 Spectral resolution: Measuring the CRMs. The maximum absorbance values were read at closest to 268.7nm and the minimum absorbance values were read at closest 267.0 nm. Refer to European Pharmacopoeia V.6.19.3 1984
2. N/A = not available.
3. Uncertainty of Measurement: The reported uncertainty of measurement was based on standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%.
4. This result of calibration was found accurate as shown on date and place of calibration only.
5. This report will certify of calibrated equipment only.

- End of Report -



Certificate of Calibration

Certificate No.: WK2411-404-43

Page 1 of 2

Customer : Ecotech Water Co., Ltd.
20 Soi Kheharomklao 74 Yaek 6, Ratphatthana,
Saphansung, Bangkok 10240

Instrument : Block Digestor
Manufacturer : BIOBASE
Model : BKD-88
Serial No. : XZL8B-202108-116
Identity No. : N/A
Range : 380 °C
Resolution : 1 °C
Calibration Method : CP-WK-T02

Ambient Temperature : (25 ± 2) °C
Humidity : (50 ± 15) %RH
Received Date : 11-Nov-24
Calibrated Date : 15-Nov-24
Issued Date : 15-Nov-24
Calibrated Location : In Lab

Reference standard instruments :

<u>Instrument</u>	<u>Serial No.</u>	<u>Certificate No.</u>	<u>Due Date</u>	<u>Traceability to</u>
Data Acquisition / Switch Unit	US37029031	WK2311-302-224	28-Nov-24	WK Electric Co., Ltd.

TPA : Technology Promotion Association (Thailand-Japan)

This result calibrate was found accurate as shown on date place of calibrate only

This certificate is traceability to the International System of Unit (SI)

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence approximately 95 %

Calibrated by : Ms. Usa Phuangphiphat

Approved by :

Mr. Ratchadawut Rungravee
Authorized Signatory

This certificate may not be reproduced except in full unless permission for the reproduction has been obtained in writing from the laboratory.



Calibration Results


Certificate No. : WK2411-404-43

Page 2 of 2

Calibration Result of the Accuracy

Range : 380 °C

Resolution : 1 °C

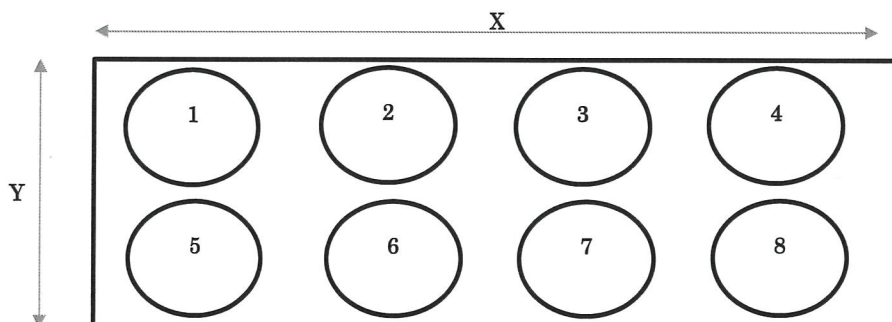

Drawing Position

X = 4

Y = 2

Unit : °C

UUC Setting	UUC Reading	Measured Temperature (°C) @ Thermocouple No. (Thermocouple No. 8 is REF.)								Uncertainty (± °C)
		1	2	3	4	5	6	7	8	
380	380	359.85	359.98	358.44	359.62	360.25	360.03	360.28	362.71	1.5

Calibration Point	UUC Setting	Standard Reading	Temperature Stability (±)	Temperature Uniformity	Overall Variation
380	380	360.15	0.50	4.55	4.58

Temperature uniformity : The maximum difference of measured temperatures at any sensors and measured temperature at the reference location which are observed at the same time or at close observation time as possible to determine the temperature pattern or homogeneity within the chamber at steady-state conditions.

Temperature stability : The one - half of greatest maximum difference of measured temperature at any one sensor, for at least half an hour after reaching steady state or after one achieved complete cycle of control whichever comes first.

Overall Variation : the difference of the maximum and the minimum measured temperatures throughout observation time.

Record time : Start time record after t₀ Average* : The average of 30 values.

Uncertainty : The report uncertainty of measurement were excluded uniformity and stability.

* UUC = Unit Under Calibrated

Note: " * " mean not accreditation

This certificate may not be reproduced except in full unless permission for the reproduction has been obtained in writing from the laboratory.

**** End of Certificate****



Certificate of Calibration

Certificate No.: WK2411-404-43

Page 1 of 2

Customer : Ecotech Water Co., Ltd.
20 Soi Kheharomklao 74 Yaek 6, Ratphatthana,
Saphansung, Bangkok 10240

Instrument : Block Digestor
Manufacturer : BIOBASE
Model : BKD-88
Serial No. : XZL8B-202108-116
Identity No. : N/A
Range : 380 °C
Resolution : 1 °C
Calibration Method : CP-WK-T02

Ambient Temperature : (25 ± 2) °C
Humidity : (50 ± 15) %RH
Received Date : 11-Nov-24
Calibrated Date : 15-Nov-24
Issued Date : 15-Nov-24
Calibrated Location : In Lab

Reference standard instruments :

<u>Instrument</u>	<u>Serial No.</u>	<u>Certificate No.</u>	<u>Due Date</u>	<u>Traceability to</u>
Data Acquisition / Switch Unit	US37029031	WK2311-302-224	28-Nov-24	WK Electric Co., Ltd.

TPA : Technology Promotion Association (Thailand-Japan)


This result calibrate was found accurate as shown on date place of calibrate only

This certificate is traceability to the International System of Unit (SI)

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence approximately 95 %

Calibrated by : Ms.Usa Phuangphiphat

Approved by :


Mr. Ratchadawut Rungravee
Authorized Signatory

This certificate may not be reproduced except in full unless permission for the reproduction has been obtained in writing from the laboratory.



Calibration Results


Certificate No. : WK2411-404-43

Page 2 of 2

Calibration Result of the Accuracy

Range : 380 °C

Resolution : 1 °C

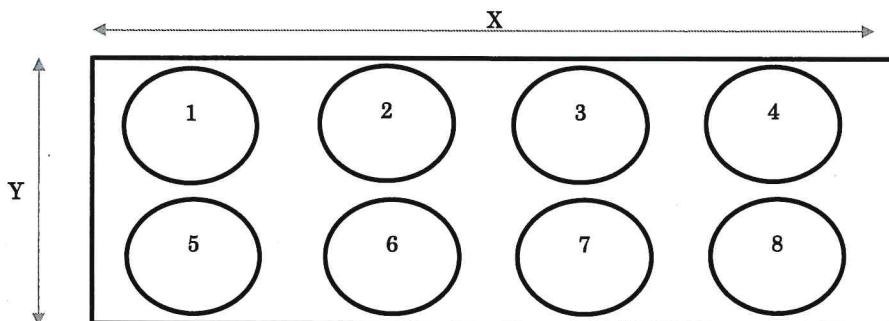

Drawing Position

X = 4

Y = 2

Unit : °C

UUC Setting	UUC Reading	Measured Temperature (°C) @ Thermocouple No. (Thermocouple No. 8 is REF.)								Uncertainty (± °C)
		1	2	3	4	5	6	7	8	
380	380	359.85	359.98	358.44	359.62	360.25	360.03	360.28	362.71	1.5

Calibration Point	UUC Setting	Standard Reading	Temperature Stability (±)	Temperature Uniformity	Overall Variation
380	380	360.15	0.50	4.55	4.58

Temperature uniformity : The maximum difference of measured temperatures at any sensors and measured temperature at the reference location which are observed at the same time or at close observation time as possible to determine the temperature pattern or homogeneity within the chamber at steady-state conditions.

Temperature stability : The one - half of greatest maximum difference of measured temperature at any one sensor, for at least half an hour after reaching steady state or after one achieved complete cycle of control whichever comes first.

Overall Variation : the difference of the maximum and the minimum measured temperatures throughout observation time.

Record time : Start time record after t₁ Average* : The average of 30 values.

Uncertainty : The report uncertainty of measurement were excluded uniformity and stability.

* UUC = Unit Under Calibrated

Note: " * " mean not accreditation

This certificate may not be reproduced except in full unless permission for the reproduction has been obtained in writing from the laboratory.

**** End of Certificate****