

ภาคผนวก จ

ใบรับรองการสอบเทียบเครื่องมือ



right solutions.
right partner.

รายการเครื่องมือที่ใช้ในการวิเคราะห์ / ทดสอบ

Sample Name	Parameter	Equipment Name	ID No.	Calibrated Date	Next Cal	Freq. Calibrate (Months)
Songkhla Lab	BOD	Incubator	SGK_CL0028	10-Jan-25	10-Jul-26	18
Songkhla Lab	BOD	DO/BOD Analyser	SGK_CL0073	21-May-24	21-Nov-25	18
Songkhla Lab	COD	COD Reactor	SGK_CL0085	15-Jan-25	15-Jan-26	12
Songkhla Lab	COD	Spectrophotometer	SGK_CL0100	25-Dec-24	25-Dec-25	12
Songkhla Lab	pH at 25 °C	pH meter	SGK_CL0030	19-Oct-24	19-Apr-26	18
Songkhla Lab	Oil & Grease	Electronic Top-Loading Balance	SGK_CL0045	10-Jan-25	10-Jan-26	12
Songkhla Lab	Oil & Grease	Oven	SGK_CL0024	19-Oct-24	19-Apr-26	18
Songkhla Lab	Oil & Grease	Water Bath	SGK_CL0035	10-Jan-25	10-Jul-26	18
Songkhla Lab	Total Dissolved Solids 180°C	Electronic Top-Loading Balance	SGK_CL0045	10-Jan-25	10-Jan-26	12
Songkhla Lab	Total Dissolved Solids 180°C	Oven	SGK_CL0024	19-Oct-24	19-Apr-26	18
Songkhla Lab	Total Suspended Solids	Electronic Top-Loading Balance	SGK_CL0045	10-Jan-25	10-Jan-26	12
Songkhla Lab	Total Suspended Solids	Oven	SGK_CL0024	19-Oct-24	19-Apr-26	18
Ambient	Total Hydrocarbon	DRYCAL FLOWMETER	BKK_FS0614	9-Sep-24	9-Sep-25	12
Ambient	Total Hydrocarbon	DRYCAL FLOWMETER	BKK_FS0619	9-Sep-24	9-Sep-25	12
Ambient	Total Hydrocarbon	Air Sampling Pump	CHM_FS0062	14-May-25	14-Aug-25	3
Ambient	Total Hydrocarbon	Air Sampling Pump	CHM_FS0063	14-May-25	14-Aug-25	3
Ambient	Total Hydrocarbon	Air Sampling Pump	CHM_FS0066	14-May-25	14-Aug-25	3
Ambient	Total Hydrocarbon	Total Hydrocarbon Analyzer	BKK_FS1068	18-Jun-25	18-Jun-26	12
Ambient	Volatile Organic Compounds	GC-MSD	RYG_EN0136	5-Jan-24	4-Jul-25	18
Ambient	Wind Speed / Wind Direction	Wind Speed / Wind Direction	BKK_FS0887	4-Jan-24	4-Jul-25	18
Ambient	Wind Speed / Wind Direction	Wind Speed / Wind Direction	BKK_FS0888	4-Jan-24	4-Jul-25	18
Ambient	Wind Speed / Wind Direction	Wind Speed / Wind Direction	BKK_FS0909	28-Jun-24	28-Dec-25	18

CALIBRATION CERTIFICATE

Issued Date : 13-Jan-2025

Certificate No. : 25TH0226

CSR No. : A101/05028

Page. : 1 of 3

Customer : ALS Laboratory Group (Thailand) Co., Ltd
114/1 Moo 8, Karnchanawanich Rd. Tambon, Ban Phru,
Amphoe Hat Yai, Songkhla, 90250

Calibration Place : Customer Laboratory

Instrument Name : Incubator

Manufacturer : Memmert

Model : ICP750

Serial No. : F816.0063

ID No. : SGK_CL0028


Resolution : 0.1 °C

Received Date : 10-Jan-2025

Calibrated Date : 10-Jan-2025

Ambient Temperature : (30 ± 10) °C

Relative Humidity : (50 ± 30) %

REVIEW BY	
APPROVED BY	
NEXT CAL. DATE 10/7/26	

Calibration Method Used :

This instrument was calibrated using the Calibration In - house method : SCAL.WI.012 based on GLA - 20


The Southern Calibration Service Co.,Ltd.calibration control system complies with requirement of ISO/IEC 17025:2017

Traceability of measurement :

This Certificate is traceable to the International and /or national standards which realize the units of measurement according to the International System of Unit (SI) through :

- TISTR : Thailand Institute of Scientific and Technological Research

Calibrated by : Ibrorhim Saleemin

Approved by : 

Imron Rattanaylum / Technical Manager



The uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written approval of Southern Calibration Service Co., Ltd.

Details of Calibration

1. Reference Standard Equipment Used:

Equipment	Model	Serial No.	Cert. no.	Due Date
Data Acquisition/Switch Unit	34970A	MY58009813	PSL-T0707-1/67	22-May-2025


2. The results reported in this certificate refer to the condition of the instrument on the date of calibration and carry no implication regarding the longterm stability of instrument.

3. This certificate is not certified any commercial transaction

4. Condition of Item : normal condition , no indication for any damage or malfunction

Result of Calibration : (☒) Without Adjustment (☐) After Adjustment

1. Sensor Installation Diagram

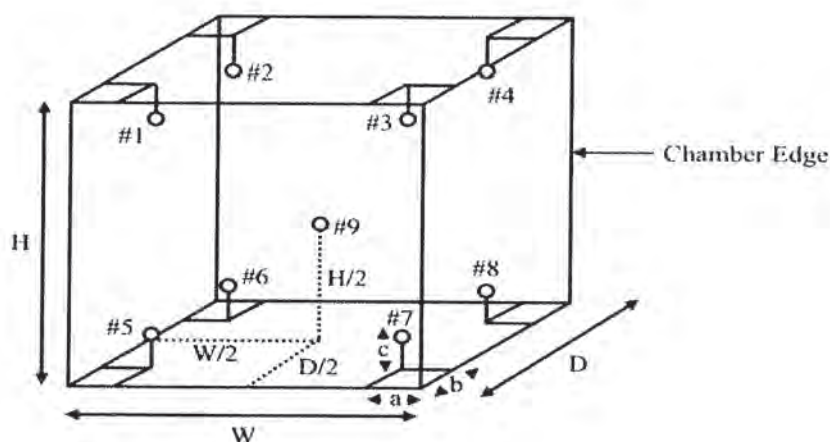

Sensor Installation Details

a = 5.0 cm
b = 5.0 cm
c = 5.0 cm

Dimension of the chamber

W = 104.0 cm
H = 120.0 cm
D = 60.0 cm

Result of Calibration :

2. Temperature Measurement Accuracy Test

The measurement results of the Incubator and associates are reported in the manner as shown below

Cal point (°C)	Measured Standard Temperature At Spread Locations (°C)									Uncertainty (± °C)
	#1	#2	#3	#4	#5	#6	#7	#8	Ref. 9	
20	20.03	20.23	20.37	20.34	20.32	20.03	20.19	20.31	20.06	0.38

3. Performance Result

The performance of the Incubator are reported as shown below

Cal point (°C)	UUC Setting (°C)	UUC Reading (°C)	Temperature Stability (± °C)	Temperature Uniformity (°C)	Overall Variation (°C)
20	20.0	20.0	0.10	0.31	0.40

- UUC = Unit Under Calibration

The report uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

... End ...



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3 : EQUIPMENT CALIBRATION AND TESTING SERVICES


534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250


TEL. 0-2717-3000 FAX. 0-2719-9484

Certificate of Testing

Cert.No.: 24TW96

Page.: 1 of 2

Equipment :	DO Meter
Manufacturer :	YSI
Model :	5000
Serial No. :	17B101473
ID No. :	SGK_CL0073
Received Date :	17 May 2024
Test Date :	21 May 2024
Reference :	2405-0608DSC-1
Submitted by :	ALS Laboratory Group (Thailand) Co.,Ltd. Songkhla Branch. 114/1 Moo 8 Karnchanawanich Rd., T.Ban Phru, A.Hat Yai, Songkhla 90250 Thailand
Laboratory Condition :	Temperature (25 ± 5) °C Humidity (50 ± 20) %
Test Procedure :	In - house method : CP-CH9 by Comparison Technique with Azide Modification Method
Tested by :	Walalak Sirithean 
Approved by :	 Approved Signatory
() Unnophol Harachai () Ponpan Paipim (✓) Saithip Meangmai	
Issue Date :	21 May 2024

REVIEW BY 

APPROVED BY.....

NEXT CAL DATE..... 21/11/25



Cert.No.: 24TW96

Page.: 2 of 2

Condition of this result of calibration

1. Reference Standard Instruments :

This certification is traceable to the International System of Unit through the reference standards laboratory of Industrial Calibration Center, Technology Promotion Association (Thailand-Japan).

<u>Instruments</u>	<u>Serial No.</u>	<u>ID No.</u>	<u>Certificate No.</u>	<u>Due Date</u>
1. Burette	-	130BU10	23CG1172	22 Mar 2025
2. Balance	14233821	110RC001	23MM405	16 July 2024

2. Standard Material :-

<u>Material</u>	<u>Manufacturer</u>	<u>Lot.No.</u>	<u>Assay</u>
Sodium Thiosulfate pentahydrate	Merck	AM1763316	100.2%

Result : Dissolved Oxygen Meter Adjustment With Air 100 %

Dissolved Oxygen Probe No.: 17B100103

Titration Method (Azide Modification Method) (mg/L)	DO Meter Reading (mg/L)	Standard Deviation (mg/L)
8.18	8.18	0.0071

This report was certified only for the instrument we tested. It is allowable to use for study. Intend to use for advertising and referral purpose is prohibited. This report may not be reproduced other in full, without written approval of the laboratory.

-o0o-



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL.0-2717-3000-29 FAX.0-2719-9484



Certificate of Calibration

Cert. No.: 24LM77

Page.: 1 of 2

Equipment : DO Meter with Sensor

Manufacturer : YSI

Model : 5000-115

Serial No. : 17B101473

ID No. : SGK_CL0073

Submitted by : ALS Laboratory Group (Thailand) Co.,Ltd.
Songkhla Branch.
114/1 Moo 8 Karnchanawanich Rd.,
T.Ban Phru, A.Hat Yai,
Songkhla 90250 Thailand

Location : TPA On Site Calibration Laboratory


Received Order : 17 May 2024


Calibrated Date : 27 May 2024

Ambient Temperature : (26 ± 10) °C

Relative Humidity : (50 ± 30) %

AC Line Voltage : (220 ± 22) V

Calibrated by : Khit Ruttanaprapachai


Approved by : 
Approved Signatory

() Ponpan Paipim
() Suwit Imjai
(✓) Kunchit Promprat

Issue Date : 28 May 2024

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3: Equipment Calibration and Testing Services.



Equipment : DO Meter with Sensor
Condition As-Received : Used Item
Reference : 2405-0608DSC-2
Procedure Used :-

Cert. No.: 24LM77
Page.: 2 of 2

Calibration were conducted using in-house calibration procedure CP-OT01 according to comparison with Industrial Platinum Resistance Thermometer (IPRT) into Temperature Bath.

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

<u>Instrument</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Traceable</u>	<u>Due Date</u>
1) Digital Thermometer	2188080	23I1216	TPA	11 Oct 2024

2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certification is traceable to the International System of Unit.

Remark : TPA : Technology Promotion Association (Thailand - Japan)

Result of Calibration :- (*) Without Adjustment

Function : Temperature measurement.

This instrument was connected with temperature sensor, S/N.: 17B100103

<u>Calibration Point</u> (°C)	<u>Immersion Depth</u> (mm)	<u>Standard Temperature</u> (°C)	<u>UUC* Reading</u> (°C)	<u>Error</u> (°C)	<u>Uncertainty</u> (± °C)	<u>Coverage Factor</u> <i>k</i>
20.00	60	20.005	19.79	-0.215	0.15	2.00

UUC* : Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-



Certificate of Calibration

Cert. No.: 25TM156

Page.: 1 of 3

Equipment : COD Reactor
Manufacturer : Hach
Model : DRB200
Serial No. : 21120C1313
ID No. : SGK_CL0085

REVIEW BY [Redacted]

APPROVED BY [Redacted]

NEXT CAL DATE..... 15/01/26

Submitted by : ALS Laboratory Group (Thailand) Co.,Ltd.
(Songkhla Branch)
Kamchanawanich Rd., T.Ban Phru,
A.Hat Yai, Songkhla 90250 Thailand
Location : Chemistry Lab

Received Order : 15 January 2025
Calibration Date : 15 - 16 January 2025
Ambient Temperature : (26 ± 10) °C
Relative Humidity : (50 ± 30) %
AC Line Voltage : (220 ± 22) V

Calibrated by : Uthen Kankawi

Approved by :

[Redacted Signature]
Approved Signatory

() Chakrit Waewwanjua
(✓) Suwit Imjai
() Kunchit Promprat

Issue Date : 06 February 2025

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Calibration and Testing Equipment Services.



Equipment : COD Reactor
Condition As-Received : Used Item
Reference : 2501-0343OC-2
Procedure Used :-

Cert. No.: 25TM156
Page.: 2 of 3

As agreed with customer the calibration was performed using in-house calibration method according to directed measurement method with Data Acquisition which connected with Thermocouple Type T.

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

<u>Instrument</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Traceable</u>	<u>Due Date</u>
1) Data Acquisition	MY44073381	23LM95	TPA	19 Jun 2024

2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certification is traceable to the International System of Unit.


Remark : TPA : Technology Promotion Association (Thailand-Japan), NSC-ONSC Accredited No. Calibration 0008

Result of Calibration :- (*) Without Adjustment

Function of UUC* : Temperature Source

Heat transfer medium used : Alumina Calcined

Environment during calibration		
	Beginning	Finished
Temp.(°C)	22	22
REL.Humi.(%)	56	55
AC Supply (Volt)	225	225

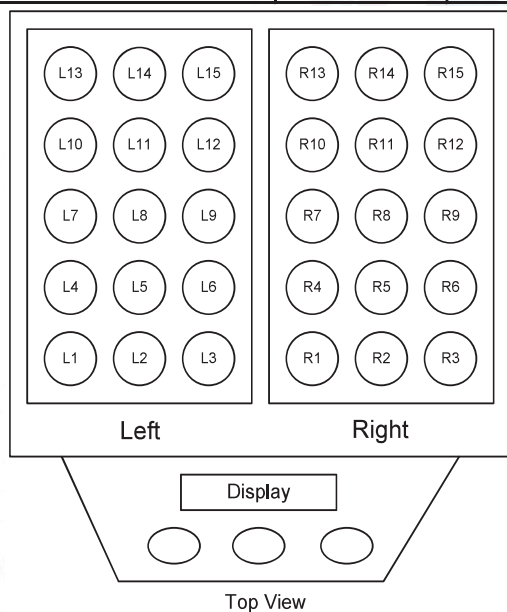

Left		Right	
Position	ID No. of Sensor	Position	ID No. of Sensor
L1	23-01TC-01	R1	23-01TC-01
L2	23-01TC-02	R2	23-01TC-02
L3	23-01TC-03	R3	23-01TC-03
L4	23-01TC-04	R4	23-01TC-04
L5	23-01TC-05	R5	23-01TC-05
L6	23-01TC-06	R6	23-01TC-06
L7	23-01TC-07	R7	23-01TC-07
L8	23-01TC-08	R8	23-01TC-08
L9	23-01TC-09	R9	23-01TC-09
L10	23-01TC-10	R10	23-01TC-10
L11	23-01TC-01	R11	23-01TC-01
L12	23-01TC-02	R12	23-01TC-02
L13	23-01TC-03	R13	23-01TC-03
L14	23-01TC-04	R14	23-01TC-04
L15	23-01TC-05	R15	23-01TC-05



Equipment : COD Reactor
Condition As-Received : Used Item
Reference : 2501-0343OC-2
Result of Calibration :- (*) Without Adjustment
Function of UUC* : Temperature Source
Calibration Point : 150 °C

Cert. No.: 25TM156

Page.: 3 of 3

UUC* Setting (°C)	UUC* Reading (°C)	Measured Temperature (°C)						Temperature stability (± °C)	Uncertainty (± °C)	Coverage Factor <i>k</i>
		Position								
		Left			Right					
150	150	L13	L14	L15	R13	R14	R15	Left 0.11	1.1	2
		149.407	149.739	149.671	148.510	148.840	148.458			
		L10	L11	L12	R10	R11	R12			
		149.910	150.069	150.171	148.894	148.931	148.753			
		L7	L8	L9	R7	R8	R9			
150	150	150.880	150.841	151.199	150.289	150.358	150.147	Right 0.11		
		L4	L5	L6	R4	R5	R6			
		150.618	150.843	151.109	150.350	150.273	149.820			
		L1	L2	L3	R1	R2	R3			
		150.229	150.688	150.838	150.094	150.115	149.792			

Average* : The average of 30 values in each position.

Temperature stability : One-half of the greatest maximum difference of measured temperature at any one sensor.

UUC* : Unit Under Calibration

Note : The reported uncertainty of measurement was included stability and excluded uniformity .

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-



SCIMET Co., Ltd.

1194 Soi Wachirathamsathit 57, Bangchak,
Phrakhanong, Bangkok 10260 Thailand
Email:scimet2022@gmail.com, Tel: 02 460 9239
https://www.scimet.co.th



Certificate No. C07240192

Calibration Certificate

Equipment: SPECTROPHOTOMETER

Model: DR 3900

Serial No.(or ID): 2403637

Manufacturer: HACH

Condition: New

Job No.: KSMT2403543

Received Date: 25 December 2024

Issued Date: 25 December 2024

Page: 1 of 3

Customer

ALS Laboratory Group (Thailand) Co., Ltd
114/1 Moo 8, Karnchanawanich Rd.T. Ban Phru, A Hatyai, Songkhla 90250

Calibration Place

Hach (Thailand) Limited.
Branch 00001, Building D Room No. D3 11, 3rd Floor, No. 735/4, Srinakarin Road,
Pattanakarn, Suanluang, Bangkok 10250 Thailand.

Calibration Date

25 December 2024

Environment Condition

Temperature: 22.2 °C \pm 0.5 °C

Humidity: 59.2 %RH \pm 2.3 %RH

The Method used

In-house method, WI07, based on ASTM E 275-08 and
ASTM E 387-04

Traceability

This certificate is traceable to the CRM maintained by National Institute
of Standards and Technology (NIST) through Starna Scientific Limited.

The standard for Wavelength Certificate No. 108691 and 108692

The standard for Photometric Certificate No. 109010 , 114655

This certificate is issued the units of
measurement according to the International
System of Units (SI). It provides traceability
of measurement to international or national
standard or other recognized national
standard laboratories.

The measurement uncertainty stated is
the expanded uncertainty which is obtained
from the standard uncertainty multiplied by
the coverage factor ($k=2$) to provide a level
of confidence of approximately 95%. It is
determined in accordance with the Guide to
Expression of Uncertainty in Measurement
(GUM).

These results may be affected by
deviations from specified conditions. The
results relate only to the items tested,
calibrated or sampled. The report shall not
be reproduced except in full without
approval of SCIMET Co., Ltd.


REVIEW BY ..	
APPROVED BY ..	
NEXT CAL. DATE ..	25 / 12 / 25



(Mr. Siwapan Srijan)
Person in charge



(Mr. Thalerngkeat Pongngam)
Authorized signatory

**Condition of reference standards Instruments / CRM:**

<u>Instruments</u>	<u>Set No.</u>	<u>Certificate No.</u>	<u>Due date</u>
Holmium Oxide Glass Reference	121512	108691	25-Jan-25
Didymium Oxide Glass Reference	119722	108692	25-Jan-25
Neutral Density Filter Reference	12276	109010 , 114655	2-Feb-25

Calibration Results:**Without Adjustment**

Wavelength Accuracy (nm), The spectral bandwidth of Std at 5 nm and UUC at 5 nm

Standard Wavelength (nm)	Unit Under Calibration (nm)	Correction (nm)	Uncertainty of Measurement (± nm)
333.67	333	0.67	0.59
361.02	361	0.02	0.59
417.80	417	0.80	0.59
441.29	441	0.29	0.59
479.88	480	-0.12	0.59
513.75	513	0.75	0.59
528.59	528	0.59	0.59
537.75	537	0.75	0.59
585.56	585	0.56	0.59
641.95	642	-0.05	0.59
684.70	685	-0.30	0.59
747.61	748	-0.39	0.59
807.04	807	0.04	0.59
879.68	880	-0.32	0.59

**Calibration Results:**

Without Adjustment

Photometric Accuracy (Absorbance)

Wavelength	Standard absorbance (Abs)	Unit Under Calibration (Abs)	Correction (Abs)	Uncertainty of Measurement(\pm Abs)
420 nm	0.0000	0.000	0.0000	0.0045
	0.2373	0.234	0.0033	0.0045
	0.5617	0.561	0.0007	0.0045
	0.7392	0.738	0.0012	0.0045
	1.0550	1.056	-0.0010	0.0045
440 nm	0.0000	0.000	0.0000	0.0045
	0.2335	0.231	0.0025	0.0045
	0.5513	0.550	0.0013	0.0045
	0.7230	0.722	0.0010	0.0045
	1.0324	1.032	0.0004	0.0045
465 nm	0.0000	0.000	0.0000	0.0045
	0.2126	0.210	0.0026	0.0045
	0.5036	0.506	-0.0024	0.0045
	0.6735	0.676	-0.0025	0.0045
	0.9615	0.965	-0.0035	0.0045
546.1 nm	0.0000	0.000	0.0000	0.0045
	0.2201	0.217	0.0031	0.0045
	0.5176	0.520	-0.0024	0.0045
	0.6930	0.694	-0.0010	0.0045
	0.9908	0.994	-0.0032	0.0045
590 nm	0.0000	0.000	0.0000	0.0045
	0.2443	0.241	0.0033	0.0045
	0.5530	0.554	-0.0010	0.0045
	0.7196	0.719	0.0006	0.0045
	1.0301	1.031	-0.0009	0.0045
635 nm	0.0000	0.000	0.0000	0.0045
	0.2646	0.261	0.0036	0.0045
	0.5370	0.538	-0.0010	0.0045
	0.6862	0.687	-0.0008	0.0045
	0.9822	0.984	-0.0018	0.0045

The End of Certificate

บริษัท ชายนีเมท จำกัด (SCIMET CO., LTD.)

1194 Soi Wachirathamsathit 57, Bangchak, Phrakhanong, Bangkok 10260 Thailand

Email: scimet2022@gmail.com, Tel: 02 460 9239

FC07-03; 30 MAY 2023

CALIBRATION CERTIFICATE

Issued Date : 22-Oct-2024

Certificate No. : 24CH0526

CSR No. : A163/08133

Page : 1 of 2

Customer : ALS Laboratory Group (Thailand) Co., Ltd
114/1 Moo 8, Karnchanawanich Rd. Tambon, Ban Phru,
Amphoe Hat Yai, Songkhla, 90250

Calibration Place : Chemical Laboratory

Instrument Name : pH meter

Manufacturer : Mettler Toledo

Model : S220

Serial No. : B625631849

ID No. : SGK_CL0030


Electrode No. : 2281592


Received Date : 19-Oct-2024

Calibrated Date : 19-Oct-2024

Ambient Temperature : $(25 \pm 3) ^\circ\text{C}$

Relative Humidity : $(55 \pm 15) \%$

REVIEW BY ... 

APPROVED BY ... 

NEXT CAL. DATE 19/4/26

Calibration Method Used :

This instrument was calibrated using the Calibration In - house method : SCAL.WI.008 based on direct measurement by using certified reference Material (CRM)

The Southern Calibration Service Co.,Ltd.calibration control system complies with requirement of ISO/IEC 17025:2017

Traceability of measurement :

This Certificate is traceable to the International and /or national standards which realize the units of measurement according to the International System of Unit (SI) through :

- CPAchem : CPAchem Ltd
- WK : WK Electric Co., Ltd.
- SCAI : Sounthern Calibration Service Co., Ltd.,

Calibrated by : Alisara Ma

Approved by :

Imron Rattanaylum / Technical Manager



The uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written approval of Southern Calibration Service Co., Ltd.

Details of Calibration

1. Reference Standard Equipment Used:

Equipment	Model	Serial No.	Cert. no.	Due Date
Standard Solution	4.000	61310674	1042701	26-Oct-2025
Standard Solution	7.000	61314184	1042700	26-Oct-2025
Standard Solution	10.01	61313804	1042702	26-Oct-2025
Temperature/Electrical Calibrator	MC2-TE	14987	WK2106-299-223	31-May-2025
Digital Thermometer With Sensor	DP-77	1.360896	24SDTH005	7-Aug-2025

2. The results reported in this certificate refer to the condition of the instrument on the date of calibration and carry no implication regarding the longterm stability of instrument.

3. This certificate is not certified any commercial transaction

4. Condition of Item : normal condition , no indication for any damage or malfunction

Result of Calibration :

1. Electrical Measurement

Applied Voltage (mV)	pH meter Reading		Correction (mV)	Uncertainty (± mV)
	(mV)	(pH)		
177.48	177.5	4.00	-0.02	0.17
0.00	0.0	7.00	0.00	0.13
-177.48	-177.5	10.00	0.02	0.17

2. Before Sample Test Measurement

Standard Buffer Solutions (pH)	pH meter Reading		Correction (pH)	Uncertainty (± pH)
	(pH)	(mV)		
4.007	3.99	178.1	0.017	0.0092
6.976	7.02	1.7	-0.044	0.019
10.009	9.96	-169.6	0.049	0.038

3. After Sample Test Measurement

Standard Buffer Solutions (pH)	pH meter Reading		Correction (pH)	Uncertainty (± pH)
	(pH)	(mV)		
4.007	3.99	177.7	0.017	0.0092
6.976	7.01	3.7	-0.034	0.019
10.009	10.00	-169.0	0.009	0.038

4. Temperature Measurement

Cal Point (°C)	Standard Temperature (°C)	UUC Reading (°C)	Correction (°C)	Uncertainty (± °C)
25	25.021	25.0	0.02	0.060

The report uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

... End ...

CALIBRATION CERTIFICATE

Issued Date : 13-Jan-2025

Certificate No. : 25MA0125

CSR No. : A101/05028

Page. : 1 of 3

Customer : ALS Laboratory Group (Thailand) Co., Ltd
114/1 Moo 8, Karnchanawanich Rd. Tambon, Ban Phru,
Amphoe Hat Yai, Songkhla, 90250

Calibration Place : Customer Laboratory
Instrument Name : Analytical Balance
Manufacturer : Sartorius
Model : MSE224S-100-DU
Serial No. : 34705158
ID No. : SGK_CL0045
Resolution : 0.0001 g
Received Date : 10-Jan-2025
Calibrated Date : 10-Jan-2025
Ambient Temperature : $(30 \pm 10) ^\circ\text{C}$
Relative Humidity : $(50 \pm 20) \%$

REVIEW BY ...

APPROVED BY ...

NEXT CAL. DATE

10/1/26

Calibration Method Used :

This instrument was calibrated using the Calibration In - house method : SCAL.WI.001 based on UKAS LAB 14 : 2015

The Southern Calibration Service Co.,Ltd.calibration control system complies with requirement of ISO/IEC 17025:2017

Traceability of measurement :

This Certificate is traceable to the International and /or national standards which realize the units of measurement
according to the International System of Unit (SI) through :

- SCaL : Sounthern Calibration Service Co., Ltd.,

Calibrated by : Hadbordee Dettawee

Approved by :

Imron Rattanaylum / Technical Manager

**The uncertainties are for a confidence probability of approximately 95%**

This certificate may not be reproduced other than in full, except with the prior written approval of Southern Calibration Service Co., Ltd.



Certificate No. : 25MA0125

CSR No. : A101/05028

Page. : 2 of 3

Details of Calibration

1. Reference Standard Equipment Used:

Equipment	Model	Serial No.	Cert. no.	Due Date
Standard Weight Set	2 mg - 1 kg	11119514/01	24SWS001	3-Jul-2025

2. The results reported in this certificate refer to the condition of the instrument on the date of calibration and carry no implication regarding the longterm stability of instrument.

3. This certificate is not certified any commercial transaction

4. Condition of Item : normal condition , no indication for any damage or malfunction

Result of Calibration : (✓) Without Adjustment () After Adjustment

1. Repeatability

Nominal Value (g)	Standard Deviation (g)
10	0.00000
20	0.00000
200	0.00000

2. Effect of tare

Nominal Value (g)	Standard Value (g)	Balance Reading (g)	Correction (g)
20	20.0000	20.0000	0.0000
40	40.0001	40.0000	0.0001
60	60.0000	60.0000	0.0000
80	80.0001	80.0000	0.0001
100	100.0000	100.0000	0.0000



Result of Calibration :

3. Off-centre loading

A mass approximately 100g was placed on a pan and moved to various position .

The balance reading obtained are given in the table.

Position					Maximum Difference (g)
1	2	3	4	5	
100.0000	100.0000	100.0000	100.0000	100.0001	0.0001



4. Departure from nominal value

Nominal Value (g)	Standard Value (g)	UUC Reading (g)	Correction (g)	Uncertainty (\pm g)	Coverage Factor (k)
0.01	0.0100	0.0100	0.0000	0.00008	2.0
0.1	0.1000	0.1000	0.0000	0.00008	2.0
0.5	0.5000	0.5000	0.0000	0.00008	2.0
1	1.0000	1.0000	0.0000	0.00008	2.0
2	2.0000	2.0000	0.0000	0.00008	2.0
5	5.0000	5.0000	0.0000	0.00009	2.0
10	10.0000	10.0000	0.0000	0.00009	2.0
20	20.0000	20.0000	0.0000	0.00009	2.0
40	40.0001	40.0000	0.0001	0.00011	2.0
50	50.0000	50.0000	0.0000	0.00013	2.0
60	60.0000	60.0000	0.0000	0.00013	2.0
80	80.0000	80.0000	0.0000	0.00016	2.0
100	100.0000	100.0001	-0.0001	0.00017	2.0
120	120.0000	120.0001	-0.0001	0.00024	2.0
140	140.0001	140.0000	0.0001	0.00024	2.0
160	160.0000	160.0000	0.0000	0.00026	2.0
180	180.0000	180.0000	0.0000	0.00029	2.0
200	200.0000	200.0000	0.0000	0.00030	2.0

- UUC = Unit Under Calibration

The report uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k, providing a level of confidence of approximately 95%

...End...



CALIBRATION CERTIFICATE

Issued Date : 22-Oct-2024

Certificate No. : 24TH4295

CSR No. : A163/08133

Page. : 1 of 3

Customer : ALS Laboratory Group (Thailand) Co., Ltd
114/1 Moo 8, Karnchanawanich Rd. Tambon, Ban Phru,
Amphoe Hat Yai, Songkhla, 90250

Calibration Place : Chemical Laboratory
Instrument Name : Hot Air Oven
Manufacturer : Memmert
Model : UF110
Serial No. : B416.3387
ID No. : SGK_CL0024
Resolution : 0.1 °C
Received Date : 19-Oct-2024
Calibrated Date : 19-Oct-2024
Ambient Temperature : (30 ± 10) °C
Relative Humidity : (50 ± 30) %

REVIEW BY	
APPROVED BY	
NEXT CAL. DATE	19/04/2026

Calibration Method Used :

This instrument was calibrated using the Calibration In - house method : SCAL.WI.012 based on GLA - 20

The Southern Calibration Service Co.,Ltd.calibration control system complies with requirement of ISO/IEC 17025:2017

Traceability of measurement :

This Certificate is traceable to the International and /or national standards which realize the units of measurement according to the International System of Unit (SI) through :

- TISTR : Thailand Institute of Scientific and Technological Research

Calibrated by : Ibrrorhim Saleemin

Approved by :

Imron Rattanaylum / Technical Manager



The uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written approval of Southern Calibration Service Co., Ltd.

Details of Calibration

1. Reference Standard Equipment Used:

Equipment	Model	Serial No.	Cert. no.	Due Date
Data Acquisiton/Switch Unit	34970A	MY58009813	PSL-T0707-1/67	22-May-2025

2. The results reported in this certificate refer to the condition of the instrument on the date of calibration

and carry no implication regarding the longterm stability of instrument.

3. This certificate is not certified any commercial transaction


4. Condition of Item : normal condition , no indication for any damage or mulfunction

Result of Calibration .:

(✓) Without Adjustment

() After Adjustment

1. Sensor Installation Diagram

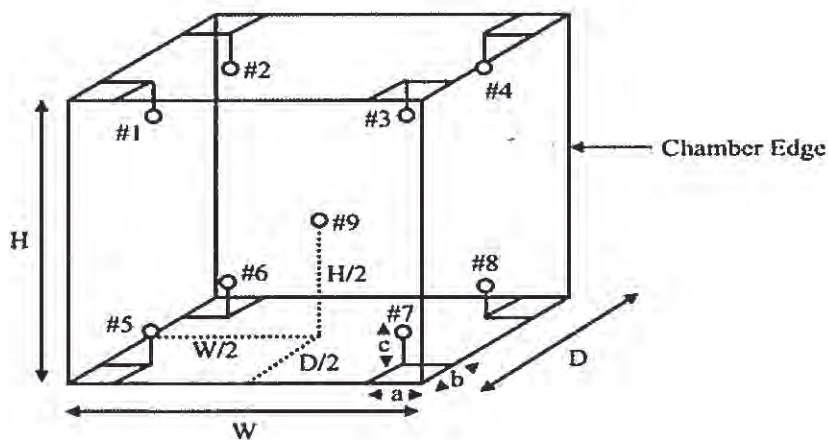

Sensor Installation Details

a = 5.0 cm

b = 5.0 cm

c = 5.0 cm

Dimension of the chamber

W = 55.0 cm

H = 48.0 cm

D = 40.0 cm

Result of Calibration :

2. Temperature Measurement Accuracy Test

The measurement results of the Hot Air Oven and associates are reported in the manner as shown below

Cal point (°C)	Measured Standard Temperature At Spread Locations (°C)									Uncertainty (± °C)
	#1	#2	#3	#4	#5	#6	#7	#8	Ref. 9	
40	40.36	40.40	40.51	40.43	40.05	40.24	40.09	40.14	39.75	0.38
70	70.27	70.30	70.45	70.24	70.24	70.43	70.29	70.30	69.95	0.36
103	102.94	102.90	103.55	102.96	103.22	103.14	103.10	103.01	102.88	0.36
104	104.15	103.99	104.27	104.06	104.09	104.23	104.26	104.15	103.90	0.36
105	105.04	104.90	105.05	104.87	104.91	104.80	104.82	104.98	104.70	0.36
180	179.19	178.93	179.82	179.10	179.27	179.68	179.12	179.73	179.12	0.41

3. Performance Result

The performance of the Hot Air Oven are reported as shown below

Cal point (°C)	UUC Setting (°C)	UUC Reading (°C)	Temperature Stability (± °C)	Temperature Uniformity (°C)	Overall Variation (°C)
40	40.0	40.0	0.20	0.84	0.84
70	70.0	70.0	0.10	0.59	0.59
103	103.0	103.0	0.20	0.73	0.74
104	104.0	104.0	0.20	0.47	0.56
105	105.0	105.0	0.20	0.44	0.46
180	180.0	180.0	0.50	0.86	1.11

- UUC = Unit Under Calibration

The report uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

... End ...

CALIBRATION CERTIFICATE

Issued Date : 13-Jan-2025

Certificate No. : 25TH0227

CSR No. : A101/05028

Page. : 1 of 3

Customer : ALS Laboratory Group (Thailand) Co., Ltd
114/1 Moo 8, Karnchanawanich Rd. Tambon, Ban Phru,
Amphoe Hat Yai, Songkhla, 90250

Calibration Place : Customer Laboratory

Instrument Name : Liquid Bath

Manufacturer : Memmert

Model : WNE29

Serial No. : L616.0538

ID No. : SGK_CL0035

Resolution : 0.1 °C

Received Date : 10-Jan-2025

Calibrated Date : 10-Jan-2025

Ambient Temperature : (30 ± 10) °C

Relative Humidity : (50 ± 30) %

REVIEW BY	[Redacted]
APPROVED BY	[Redacted]
NEXT CAL. DATE	10/7/26

Calibration Method Used :

This instrument was calibrated using the Calibration In - house method : SCAL.WI.014 based on ASTM E 715 : 1980 (reapproved 2001)

The Southern Calibration Service Co.,Ltd.calibration control system complies with requirement of ISO/IEC 17025:2017

Traceability of measurement :

This Certificate is traceable to the International and /or national standards which realize the units of measurement according to the International System of Unit (SI) through :

- TISTR : Thailand Institute of Scientific and Technological Research

Calibrated by : Ibrorhim Saleemin

Approved by :

Imron Rattanaylum / Technical Manager



The uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written approval of Southern Calibration Service Co., Ltd.

Details of Calibration

1. Reference Standard Equipment Used:

Equipment	Model	Serial No.	Cert. no.	Due Date
Data Acquisition/Switch Unit	34970A	MY58009813	PSL-T0707-1/67	22-May-2025

2. The results reported in this certificate refer to the condition of the instrument on the date of calibration

and carry no implication regarding the longterm stability of instrument.

3. This certificate is not certified any commercial transaction


4. Condition of Item : normal condition , no indication for any damage or malfunction

Result of Calibration :

(☒) Without Adjustment

(☐) After Adjustment

1. Sensor Installation Diagram

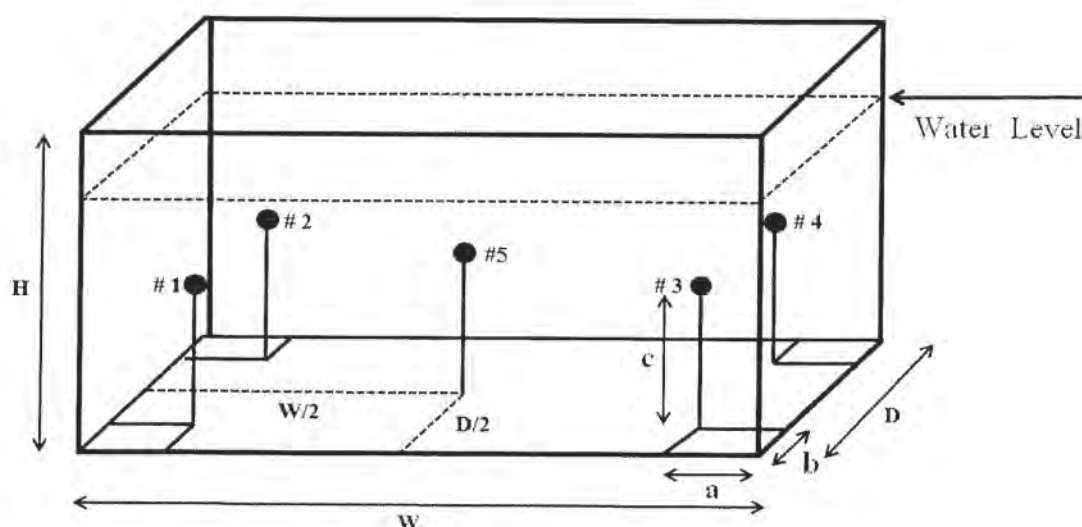

Sensor Installation Details

a = 5 cm

b = 5 cm

c = 5 cm

Dimension of the chamber

W = 59.0 cm

H = 14.0 cm

D = 35.0 cm

Result of Calibration :

2. Temperature Measurement Accuracy Test

The measurement results of the Liquid Bath and associates are reported in the manner as shown below

Cal point (°C)	Measured Standard Temperature At Spread Locations (°C)					Uncertainty (± °C)
	#1	#2	#3	#4	Ref.5	
80	80.05	80.07	79.98	80.05	80.06	0.17

3. Performance Result

The performance of the Liquid Bath are reported as shown below

Cal point (°C)	UUC Setting (°C)	UUC Reading (°C)	Temperature Stability (± °C)	Temperature Uniformity (°C)	Overall Variation (°C)
80	80.0	80.0	0.20	0.17	0.26

- UUC = Unit Under Calibration

The report uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

... End ...

Certificate of Calibration

Customer

Name : ALS Laboratory Group Thailand Co., Ltd.
Address : 104 Soi Phatthanakan 40, Phatthanakan Road, Suan Luang,
Bangkok 10250

Certificate No : 24-AFM-179

Request No : Req-2024-1987

Unit Under Calibration Details

Measurement Item : Air Flow Meter
Manufacturer : MesaLabs Accuracy : 1% of Reading
Model : Defender 510-M Sensor Model : -
Serial Number : 151114 Sensor Serial Number : -
ID : BKK_FS0614 Instrument Status : Used
Location of Calibration : LAB 4 AIR VELOCITY METER

Calibration Environment and Details

Temperature : 23 °C ± 3 °C
Humidity : 55 %RH ± 20 %RH
Barometric Pressure : 1013 hPa ± 10 hPa
Received Date : 30 August 2024
Calibration Date : 9 September 2024
Calibration Procedure : In-house method CP-AFM-01 by Comparison technique with Standard Primary Flow Calibrator

REVIEW BY	
APPROVED BY	
NEXT CAL. DATE	9/9/25


Reference Standard	Model	Serial Number	Traceable	Due Calibration
Air Flow Meter	Gilibrator 3 Low flow	18501010006	Sensidyne	6 August 2025
Air Flow Meter	Gilibrator 3 Standard flow	19031011003	Sensidyne	2 August 2025
Temperature meter	GT 11	08000057	Qreborn	1 March 2025
Pressure meter	CPG2400	41000KDU/651882	TPA	9 November 2024


Traceability :

This Certificate is traceable to SI Unit through Sensidyne A2LA Accreditation No. 3943.01

Note :

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor $k = 2$, providing a level of confidence approximately 95 %.

Calibration By : 
Mr. Noppadon Luangart
Service Calibration Engineer

Approved By : 
Mr. Pacit Mathavorn
Calibration Engineer Supervisor

Issue Date : 9 September 2024

Certificate No : 24-AFM-179

Request No : Req-2024-1987

Result of Calibration : Without Adjustment

Temperature (°C)	Pressure (kPa)	STD (cc/min)	UUC (cc/min)	Error (cc/min)	Uncertainty (cc/min)	MPE (cc/min)	Result
24.70	100.95	100	100.41	0.4	2.8	1.0	N/A
24.90	100.90	502	500.47	-1.5	7.1	5.0	N/A
24.90	100.97	1003	1001.3	-2	14	10.0	N/A
25.00	100.92	2014	2009.9	-4	29	20.1	N/A
25.20	101.03	3043	3058.3	15	44	30.4	N/A
25.30	101.10	4043	4005.1	-38	57	40.4	N/A
25.50	101.15	5052	5003.9	-48	74	50.5	N/A

Note

STD : Standard UUC : Unit Under Calibration

- UUC Reference Condition : At atmospheric pressure and room temperature condition

- Flow Rate was corrected for non-standard operating condition by using equation :

$$Q_{meas} = Q_{ref} \times \frac{P_{ref}}{P_{meas}} \times \frac{T_{meas}}{T_{ref}}$$

where Q = Flow Rate P = Absolute Pressure T = Absolute Temperature

Meas = Measurement Condition ref = Standard Condition

* Indicates non accredited

MPE = Maximum Permissible Error (Specified in Manufacturer's Specifications)

N/A = Not Available, Customer does not require a statement of conformity.

Certificate No : 24-AFM-179

Request No : Req-2024-1987

Decision Rule for Statements of Conformity


The standard decision rule employed for the statements of conformity to each calibration result will be applied using ILAC-G8:09/2019; Guidelines on the Reporting of Compliance with Specification as following Fig. and statements

Pass = The measurement result plus the expanded uncertainty with a 95% coverage probability were within the limit.

Passⁱ = The measurement result was within the limit. However, a portion of the expanded uncertainty of measurement at 95% exceeds the limit.

Failⁱ = The measurement result was out of the limit. However, a portion of the expanded uncertainty of measurement at 95% is within the limit.

Fail = The measurement result plus the expanded uncertainty with a 95% coverage probability were outside the limit.

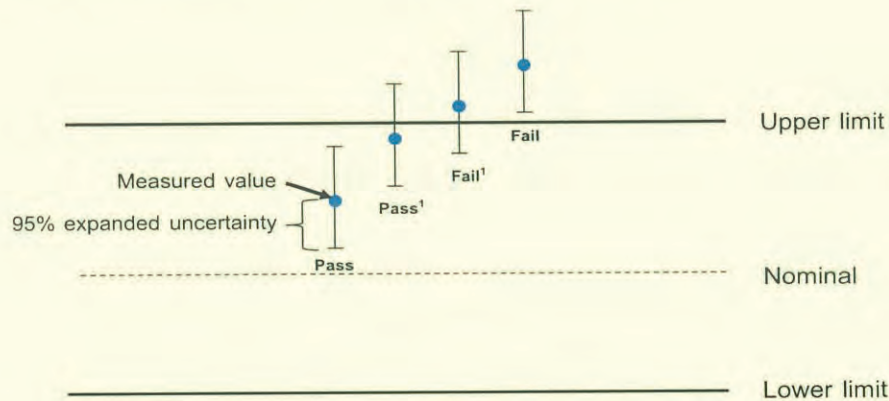

End of Certificate

Certificate of Calibration

Customer

Name : ALS Laboratory Group Thailand Co., Ltd.
Address : 104 Soi Phatthanakan 40, Phatthanakan Road, Suan Luang,
Bangkok 10250

Certificate No : 24-AFM-177

Request No : Req-2024-1862

Unit Under Calibration Details

Measurement Item : Air Flow Meter

Manufacturer : Bios

Accuracy : 1% of Reading

Model : Defender 510-L

Sensor Model : -

Serial Number : 130026

Sensor Serial Number : -

ID : BKK_FS0619

Instrument Status : Used

Location of Calibration : LAB 4 AIR VELOCITY METER

Calibration Environment and Details

Temperature : 23 °C ± 3 °C


Humidity : 55 %RH ± 20 %RH

Barometric Pressure : 1013 hPa ± 10 hPa

Received Date : 22 August 2024

Calibration Date : 9 September 2024

Calibration Procedure : In-house method CP-AFM-01 by Comparison technique with Standard Primary Flow Calibrator

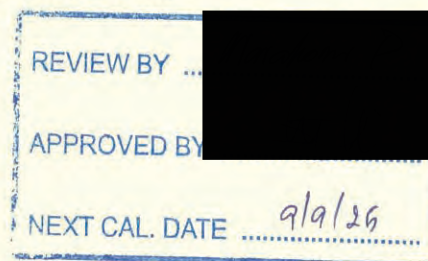

Reference Standard	Model	Serial Number	Traceble	Due Calibration
Air Flow Meter	Gilibrator 3 Low flow	18501010006	Sensidyne	6 August 2025
Air Flow Meter	Gilibrator 3 Standard flow	19031011003	Sensidyne	2 August 2025
Temperature meter	GT 11	08000057	Qreborn	1 March 2025
Pressure meter	CPG2400	41000KDU/651882	TPA	9 November 2024

Traceability :

This Certificate is traceable to SI Unit through Sensidyne A2LA Accreditation No. 3943.01

Note :

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor $k = 2$, providing a level of confidence approximately 95 %.

Calibration By :

Mr. Noppadon Luangart
Service Calibration Engineer

Approved By :

Mr. Pacit Mathavorn
Calibration Engineer Supervisor

Issue Date :

9 September 2024

Certificate No : 24-AFM-177

Request No : Req-2024-1862

Result of Calibration : Without Adjustment

Temperature (°C)	Pressure (kPa)	STD (cc/min)	UUC (cc/min)	Error (cc/min)	Uncertainty (cc/min)	MPE (cc/min)	Result
24.70	100.92	20	20.192	0.2	1.3	0.2	N/A
24.70	100.90	100	99.923	-0.1	2.8	1.0	N/A
24.70	100.94	201	200.7	-0.3	5.6	2.0	N/A
24.70	100.97	298	300.1	2.1	8.4	3.0	N/A
24.70	100.99	403	399.1	-4	11	4.0	N/A
24.80	101.05	482	477.6	-4.4	6.9	4.8	N/A

Note

STD : Standard UUC : Unit Under Calibration

- UUC Reference Condition : At atmospheric pressure and room temperature condition

- Flow Rate was corrected for non-standard operating condition by using equation :

$$Q_{\text{meas}} = Q_{\text{ref}} \times \frac{P_{\text{ref}}}{P_{\text{meas}}} \times \frac{T_{\text{meas}}}{T_{\text{ref}}}$$

where Q = Flow Rate P = Absolute Pressure T = Absolute Temperature

Meas = Measurement Condition ref = Standard Condition

* Indicates non accredited

MPE = Maximum Permissible Error (Specified in Manufacturer's Specifications)

N/A = Not Available, Customer does not require a statement of conformity.

Certificate No : 24-AFM-177

Request No : Req-2024-1862

Decision Rule for Statements of Conformity


The standard decision rule employed for the statements of conformity to each calibration result will be applied using ILAC-G8:09/2019; Guidelines on the Reporting of Compliance with Specification as following Fig. and statements

Pass = The measurement result plus the expanded uncertainty with a 95% coverage probability were within the limit.

Pass¹ = The measurement result was within the limit. However, a portion of the expanded uncertainty of measurement at 95% exceeds the limit.

Fail¹ = The measurement result was out of the limit. However, a portion of the expanded uncertainty of measurement at 95% is within the limit.

Fail = The measurement result plus the expanded uncertainty with a 95% coverage probability were outside the limit.

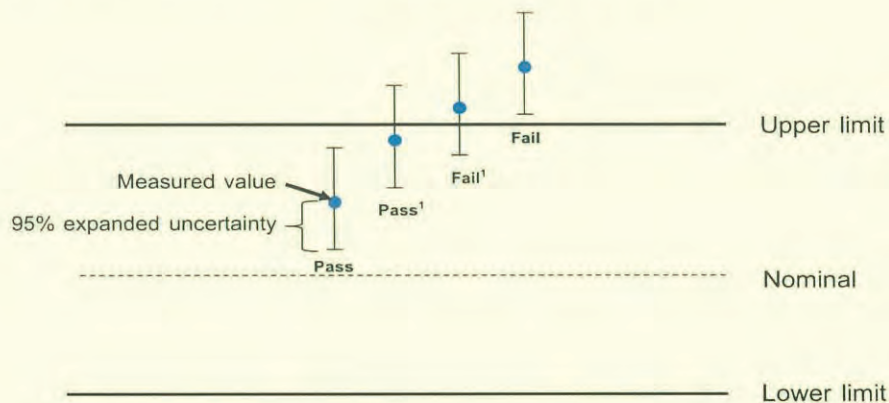

End of Certificate



Certificate of Calibration

Certificate No. C-140525-CHM_FS0062

Air Sampling Pump Detail

Equipment name : Personal Air Sampling Pump
Brand : Gilian
Model/Type : GilAir PlusEquipment ID : CHM_FS0062
Serial No. : 20191210011
Calibration Date : 14-May-25
Next calibration date : 14-Aug-25

Reference Standard Low Flow Meter

Equipment name : Air Flow Meter
Brand : MesaLabs
Model/Type : Defender 510-LEquipment ID : BKK_FS0619
Serial No. : 130026
Calibration Date : 9-Sep-24
Due Date : 9-Sep-25

Reference Standard High Flow Meter

Equipment name : Air Flow Meter
Brand : MesaLabs
Model/Type : Defender 510-MEquipment ID : BKK_FS0614
Serial No. : 151114
Calibration Date : 9-Sep-24
Due Date : 9-Sep-25

Calibration Data

Air Sampling Pump setting (cc/min)	Reference Std. Flow Reading (cc/min)			Avg. (cc/min)	%Error acceptance	Acceptable range (cc/min)			Evaluation (Pass/ Fail)
	1	2	3						
Low Flow									
20	19.3	19.1	19.3	19.2	5%	19	-	21	Passed
50	50.8	50.9	50.9	50.9	5%	48	-	53	Passed
100	99.2	99.4	100.2	99.6	5%	95	-	105	Passed
200	200.5	200.3	200.4	200.4	5%	190	-	210	Passed
High Flow									
500	501.1	503.0	500.9	501.7	3%	485	-	515	Passed
1000	1015.9	1008.2	1004.8	1009.6	3%	970	-	1030	Passed
2000	1993.0	2000.1	2002.2	1998.4	3%	1940	-	2060	Passed
2500	2502.9	2505.1	2501.0	2503.0	3%	2425	-	2575	Passed

END OF REPORT

Calibrated By: _____

(Mr.Sitthichok Taseeda)
CHM Field Services Scientist (3)

Issue date : 15-May-25

Approved By: _____

(Mr.Warakorn Pookrak)
BKK Field Services Supervisor



Certificate of Calibration

Certificate No. C-140525-CHM_FS0063

Air Sampling Pump Detail

Equipment name : Personal Air Sampling Pump
Brand : Gilian
Model/Type : GilAir PlusEquipment ID : CHM_FS0063
Serial No. : 20191210012
Calibration Date : 14-May-25
Next calibration date : 14-Aug-25

Reference Standard Low Flow Meter

Equipment name : Air Flow Meter
Brand : MesaLabs
Model/Type : Defender 510-LEquipment ID : BKK_FS0619
Serial No. : 130026
Calibration Date : 9-Sep-24
Due Date : 9-Sep-25

Reference Standard High Flow Meter

Equipment name : Air Flow Meter
Brand : MesaLabs
Model/Type : Defender 510-MEquipment ID : BKK_FS0614
Serial No. : 151114
Calibration Date : 9-Sep-24
Due Date : 9-Sep-25

Calibration Data

Air Sampling Pump setting (cc/min)	Reference Std. Flow Reading (cc/min)			Avg. (cc/min)	%Error acceptance	Acceptable range (cc/min)			Evaluation (Pass/ Fail)
	1	2	3						
Low Flow									
20	20.7	20.7	20.6	20.7	5%	19	-	21	Passed
50	50.8	50.8	50.9	50.8	5%	48	-	53	Passed
100	100.8	100.7	101.2	100.9	5%	95	-	105	Passed
200	199.2	199.5	200.2	199.6	5%	190	-	210	Passed
High Flow									
500	499.1	498.7	500.7	499.5	3%	485	-	515	Passed
1000	995.8	995.7	995.5	995.7	3%	970	-	1030	Passed
2000	1996.9	1997.6	1997.3	1997.3	3%	1940	-	2060	Passed
2500	2498.9	2501.2	2498.0	2499.4	3%	2425	-	2575	Passed

END OF REPORT

Calibrated By:

(Mr.Sitthichok Taseeda)
CHM Field Services Scientist (3)

Issue date : 15-May-25

Approved By:

(Mr.Warakorn Pookrak)
BKK Field Services Supervisor



Certificate of Calibration

Certificate No. C-140525-CHM_FS0066

Air Sampling Pump Detail

Equipment name : Personal Air Sampling Pump
Brand : Gilian
Model/Type : GilAir PlusEquipment ID : CHM_FS0066
Serial No. : 20191210015
Calibration Date : 14-May-25
Next calibration date : 14-Aug-25

Reference Standard Low Flow Meter

Equipment name : Air Flow Meter
Brand : MesaLabs
Model/Type : Defender 510-LEquipment ID : BKK_FS0619
Serial No. : 130026
Calibration Date : 9-Sep-24
Due Date : 9-Sep-25

Reference Standard High Flow Meter

Equipment name : Air Flow Meter
Brand : MesaLabs
Model/Type : Defender 510-MEquipment ID : BKK_FS0614
Serial No. : 151114
Calibration Date : 9-Sep-24
Due Date : 9-Sep-25

Calibration Data

Air Sampling Pump setting (cc/min)	Reference Std. Flow Reading (cc/min)			Avg. (cc/min)	%Error acceptance	Acceptable range (cc/min)			Evaluation (Pass/ Fail)
	1	2	3						
Low Flow									
20	20.2	20.7	20.8	20.6	5%	19	-	21	Passed
50	49.8	49.6	49.6	49.7	5%	48	-	53	Passed
100	100.5	100.7	101.0	100.7	5%	95	-	105	Passed
200	201.3	201.1	201.2	201.2	5%	190	-	210	Passed
High Flow									
500	498.7	497.5	498.2	498.1	3%	485	-	515	Passed
1000	998.0	997.2	1001.7	999.0	3%	970	-	1030	Passed
2000	2001.9	2000.9	2002.2	2001.7	3%	1940	-	2060	Passed
2500	2496.4	2498.0	2498.9	2497.8	3%	2425	-	2575	Passed

END OF REPORT
-----Calibrated By: (Mr.Sitthichok Taseeda)
CHM Field Services Scientist (3)

Issue date : 15-May-25


Approved By: (Mr.Warakorn Pookrak)
BKK Field Services Supervisor

TEST REPORT

CUSTOMER NAME	: ALS Laboratory Group (Thailand) Co., Ltd. [บริษัท เอแอลเอส แลборาทอรี กรุ๊ป (ประเทศไทย) จำกัด]						
EQUIPMENT NAME	: THC Analyzer						
MANUFACTURER	: HORIBA	MODEL	: APHA-370	SERIAL NO	: WKJON9M		
STANDARD GAS CONCENTRATION (PPM) (CH4) : 506.1 PPM				CYLINDER NO	: CC734373		
CYLINDER PRESSURE (psig) : 1,600 PSI				CERTIFIED DATE	: 12/05/2020		
CERTIFIED BY : AIRGAS				EXPIRED DATE	: 12/05/2028		

TEST RESULTS

POINT NO	TEST RESULTS						
	IDEAL	ACTUAL CH4	ERROR CH4	%ERROR CH4	ACTUAL THC	ERROR THC	%ERROR THC
ZERO	0.00	0.00	0.00	-	0.00	0.00	-
1	10.00	9.81	-0.19	-1.90	9.95	-0.05	-0.50
2	20.00	19.60	-0.40	-2.00	19.58	-0.42	-2.10
3	30.00	30.03	0.03	0.10	29.91	-0.09	-0.30
4	40.00	40.00	0.00	0.00	40.00	0.00	0.00
AVERAGE (%)				-0.95			-0.73

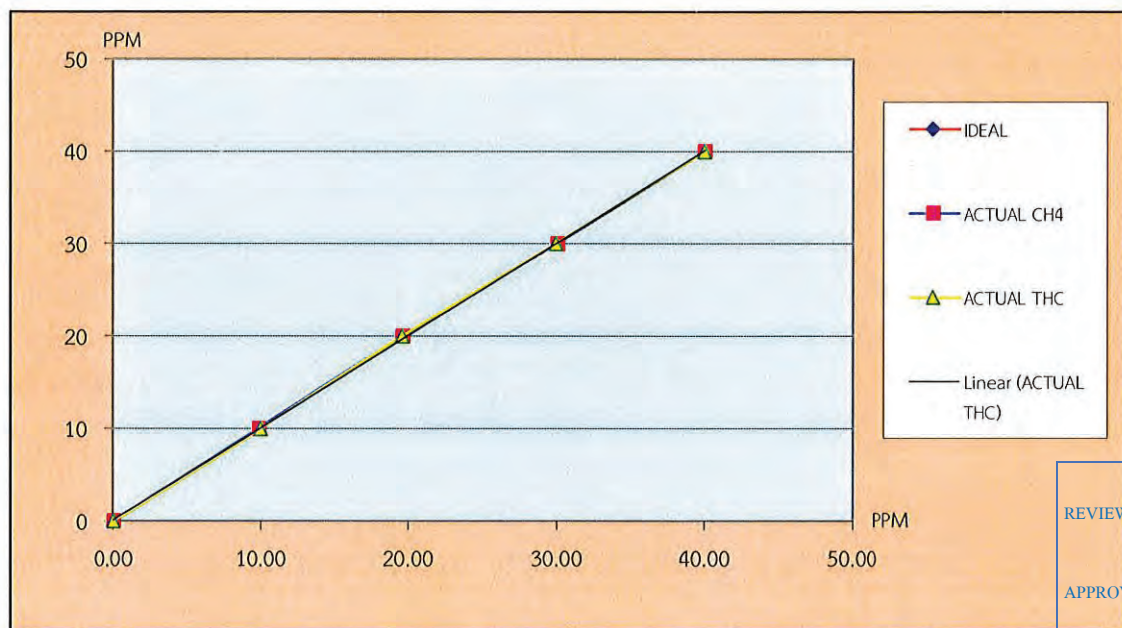

REVIEW BY ..

APPROVED BY ..

NEXT CAL DATE... 18/06/26

CALIBRATED BY :

DATE : 18/6/68

CHECKED BY :

DATE : 18/6/68

ต้องการข้อมูลทางด้านเทคนิคเพิ่มเติม : เจ้าหน้าที่ฝ่ายบริการหลังการขาย , โทร 02-868-0812 # 15,16 , E-Mail : Engineer@jiranatee.com
เลขที่ 63/14-15,67/35-36 ถนนเพชรเกษม 7,7/1 แขวงวัดท่าพระ เขตบางกอกใหญ่ กรุงเทพฯ 10600 โทร 02-8680812-13 โทรสาร 02-868-1889

CHECK LIST

CUSTOMER NAME	: ALS Laboratory Group (Thailand) Co., Ltd. [บริษัท เอแอลเอส แลบบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด]		
EQUIPMENT NAME	: THC Analyzer		
MANUFACTURER	: HORIBA	MODEL : APHA-370	SERIAL NO. : WKJON9M

TEST VALUES				
NO.	THC Analyzer (APHA - 370)	UNIT	BEFORE	AFTER
1	Signal (CH4)	mV	1.10	27.50
2	Signal (THC)	mV	0.00	31.60
3	Detector	Temp °C , Standard Value : Ambient temp+(5°Cto15°C)	30.40	48.10
		Pressure kPa , Standard Value : (Ambient/1013x100-20)±4kPa	81.20	81.00
4	Ambient	kPa current atmospheric pressure	101.70	101.60
5	Purifire	°C , Standard Value : 390 °C to 430 °C	30.30	418.70
		kPa , Normal value : 8 kPa to 25 kPa	7.20	7.20
6	NMHC	°C , Standard Value : 230 °C to 260 °C	30.10	244.20
7	DC 24 V	V , Standard Value : 24 V ± 0.5 V	24.90	24.90
8	DC 5 V	V , Standard Value : 5 V ± 0.5 V	4.90	4.90
9	Bypass (Optional)	L/min, Normal value : 0.9 L/min ± 0.3 L/min	-	-
10	Over Flow (Optional)	L/min, Standard Value : 0.8 L/min or More	-	-
11	CH4 Sampling Reading	PPM	1.33	1.95
12	NMHC Sampling Reading	PPM	0.32	0.10
13	THC Sampling Reading	PPM	1.64	2.05
14	Zero Gas CH4/THC	PPM	-0.71/-0.88	0.0/0.0
15	Span Gas	PPM	41.71/41.89	40.0/40.0
G	Gas H2/.....	20 PSI	20	20

Remark : Reference EX-EN-017-56 , Ambient HC Monitor APHA-370 Operation Manual Page #81

Remark : (Ambient temperature = 5°C to 40°C)

อาการที่ตรวจพบ

- Service Maintenance

รายละเอียดการดำเนินการ

- ทำการ Service Maintenance , ทำ Calibration Zero/Span , Multipoint

ผลการดำเนินการ

- เรียบร้อย เครื่องสามารถดำเนินการตรวจวัดได้ตามปกติ

CALIBRATED BY :



DATE : 18/6/68

CHECKED BY :

DATE : 18/6/68

ต้องการข้อมูลทางด้านเทคนิคเพิ่มเติม : เจ้าหน้าที่ฝ่ายบริการหลังการขาย , โทร 02-868-0812 # 15-16 , E-Mail : Engineer@jiranatee.com
เลขที่ 63/14-15,67/35-36 ซอยเพชรเกษม 7,7/1 ถนนเพชรเกษม แขวงวัดท่าพระ เขตบางกอกใหญ่ กรุงเทพฯ 10600 โทร 02-868-0812-13 โทรสาร 02-868-1889

Certificate of System Qualification

GC-OQ + GCMS-OQ

System ID:

RYG_EN0136

Organization Name:

ALS Laboratory Group (Thailand) Co.Ltd.

Organization Location:

616/10, Moo 5, Tambol Mae Nam Khu, Pluak Daeng, Rayong,21140, Thailand

Date:

January 5, 2024 10:53:24 AM

EQP Name:

AgilentRecommended , AgilentRecommended

EQP Revision:

GC.02.54, GCMS.02.54

Overall Qualification Status:

Pass

REVIEW BY

APPROVED BY

NEXT CAL. DATE 11/07/2025

CDS Logon Verification - GC

Logon:

chonticha.khunkaew

Overall CDS Logon Verification - GC Test Status

Pass

System Inspection and Basic Safety and Operation

Name:

7890

Setpoint Status:

Pass

Overall System Inspection and Basic Safety and Operation Test Status

Pass

Inlet Pressure Accuracy

Name:

7890

Front

SSL

Setpoint Status:

Pass

Setpoint

Actual

Inlet Pressure:

25.0

psi

25

psi

Accuracy:

0.0

psi

Agilent Recommended:

<=

1.2

Overall Inlet Pressure Accuracy Test Status

Pass

GC Oven Temperature Accuracy

Name:	7890				
Setpoint Status:	Pass				
Zone:	Oven				
	Setpoint/Actual				
Temperature:	230.0	229	°C		
Accuracy:		-1.0	°C		
Agilent Recommended:	>=	-1.0	% setpoint in K	(-5.0	°C)
	<=	1.0	% setpoint in K	(5.0	°C)
Setpoint Status:	Pass				
Zone:	Oven				
	Setpoint/Actual				
Temperature:	100.0	100.8	°C		
Accuracy:		0.8	°C		
Agilent Recommended:	>=	-1.0	% setpoint in K	(-3.7	°C)
	<=	1.0	% setpoint in K	(3.7	°C)

Overall GC Oven Temperature Accuracy Test Status

Pass

GC Oven Temperature Stability

Name:	7890				
Setpoint Status:	Pass				
	Setpoint/Average				
Temperature:	100.0	100.8167	°C		
Stability:		0.1	°C		
Agilent Recommended:	<=	0.5			

Overall GC Oven Temperature Stability Test Status

Pass

Log Amp

Tested Combination1	Front	SSL	/ External	SQ
Name:	5977B			
Setpoint Status:	Pass			
Overall Log Amp Test Status				
Pass				

RFPA

Tested Combination1	Front	SSL	/ External	SQ
Name:	5977B			
Setpoint Status:	Pass			
Amu:	1050	m/z	Drift After Five Minutes:	RFPA Voltage:
			6 mV	509 mV
Agilent Recommended:	>= -100 and <= 100		<= 1100	
Overall RFPA Test Status				
Pass				

Tune EI

Tested Combination1	Front	SSL	/ External	SQ
Name:	5977B			
Setpoint Status:	Pass			
Filament:	1			
Setpoint Status:	Pass			
Filament:	2			
Overall Tune EI Test Status				
Pass				

Scouting Run

Tested Combination1 Front SSL / External SQ

Manual Injection

Name: Not applicable

Source: EI - Extractor

Setpoint Status: Completed

Injection Volume on Column: 1.0 uL

Overall Scouting Run Status

Completed

Signal to Noise EI

Tested Combination1 Front SSL / External SQ

Name: 5977B

Source: EI - Extractor Filament: 1

Setpoint Status: Pass

Signal to Noise: 5113

Agilent Recommended: >= 1200

Source: EI - Extractor Filament: 2

Setpoint Status: Pass

Signal to Noise: 4456

Agilent Recommended: >= 1200

Overall Signal to Noise EI Test Status

Pass

NOTE: This test's 2 comment(s) and 3 deviation(s) are available in the Attachments section.

Instrument Details

Purpose

This section describes the as found system configuration.

Details

System

System ID	RYG_EN0136
Manufacturer	Agilent Technologies
Name	7890
Flow Data Input	Manual Data
Temperature Data Input	Manual Data or Other Data Logging

Tested Combination1

Injection Technique	Manual Injection
Inlet	Front
Detector	External
LTM Included?	No

Sampler 1

Manufacturer	Agilent Technologies
Type	Manual Injection
Usage	Sample Injection
Syringe Volume (µL)	10

Mainframe 1

Manufacturer	Agilent Technologies
Name	7890
Model Number	G3442B
Serial Number	CN16463238
Firmware Revision	B.02.04.3
Component ID/Asset No.	081117000236
Oven Type	Standard

Inlet 1

Manufacturer	Agilent Technologies
Name	7890
Type	SSL
Location	Front
Carrier Gas	Helium
Control Type	Electronic Pressure Control (EPC)
Purged Inlet	Yes

Detector 1

Manufacturer	Agilent Technologies
Name	Mass Spectrometer
Type	Mass Spectrometer
Location	External

Mass Spectrometer 1

Manufacturer	Agilent Technologies
Type	SQ
Name	5977B
Model Number	G7077B
Serial Number	US1701M008
Firmware Revision	5977 6.00.34
High Vacuum System	Turbo Pump
Scouting Run Standard	OFN Std
Component ID/Asset No.	081117000236

MS EI Source 1

Manufacturer	Agilent Technologies
Source Type	EI - Extractor
Number of filaments	2

Electronic Signature

Purpose

This signature page was created and published because the ACE sign-off action was executed, which is valid for the entire document, including attachments. The ACE sign-off is an electronic signature that requires two distinct identification components: unique username and personal password. The Agilent representative who has delivered this service understands the meaning and legal status of an electronic signature. As a trained official operator, the Agilent representative has a unique password and logon to access ACE and electronically sign this document. (Other e-signatures can be applied to this document using a Document Content Management or other suitable method defined in your data access and control procedures.)

Details

Full Name of Signer:	Eaknarin Puangsopa
Logged On User Name:	eaknarin_puangsopa@agilent.com
Signature Creation Date:	January 5, 2024
Reason for Signature:	Executed protocol and published this original version of document

Regulatory Disclaimer

This document provides a protocol to verify and record instrument configuration and evidence of proper operation. It has been prepared from our interpretation of applicable regulations as well as industry best practices. The document is designed to provide an important component of a complete compliance package. Validation depends upon many factors and use of this protocol alone does not assure compliance. Agilent Technologies makes no promises or representations as to its sufficiency for any specific regulatory program.

Warranty

Agilent Technologies makes no warranty of any kind to this material, including but not limited to, the implied warranties or merchantability and fitness for a particular purpose. Agilent Technologies shall not be liable for errors contained herein or for incidental or consequential damages in connection with the furnishing, performance, or use of this material.

User Name: eaknarin_puangsoa
Report Generated by Hostname: ASRYGWX074

System Id: RYG_EN0136
Print Date: January 5, 2024 10:53:25 AM

ALS_OQ_RYG_EN0136 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
January 4, 2024 10:37:31 AM	Audit	SessionCreated	Session	None
January 4, 2024 10:37:31 AM	Start	Configuration	Session	None
January 4, 2024 10:37:31 AM	Audit	Entitlement	Licensing	User is FieldEngineer and does not require an unlock code
January 4, 2024 10:39:29 AM	Audit	EqpLoaded	Session	EQP details for primary technique [Gc] - File path: [ProtocolPacks/Gc/Configurations/02.54/Gc.02.54.eqp], EQP File Name: [Gc.02.54.eqp], EQP Name: [AgilentRecommended], Protocol Revision :[Gc.02.54] EQP details for hyphenated technique [GcMs] - File path: [ProtocolPacks/GcMs/Configurations/02.54/GcMs.02.54.eqp], EQP File Name: [GcMs.02.54.eqp], EQP Name: [AgilentRecommended]
January 4, 2024 10:39:40 AM	End	Configuration	Session	None
January 4, 2024 10:39:44 AM	Start	Qualification	Session	OQ
January 4, 2024 10:39:44 AM	Start	Execution	CDS Logon Verification - GC - 7890: - Qualitative test	None
January 4, 2024 10:46:00 AM	End	Execution	CDS Logon Verification - GC - 7890: - Qualitative test	Run Count : 1

User Name: eaknarin_puangsoa
Report Generated by Hostname: ASRYGWX074

System Id: RYG_EN0136
Print Date: January 5, 2024 10:53:25 AM

ALS_OQ_RYG_EN0136 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
January 4, 2024 10:46:05 AM	Start	Execution	System Inspection and Basic Safety and Operation - 7890: - Qualitative Test - No setpoints associated	None
January 4, 2024 10:46:18 AM	End	Execution	System Inspection and Basic Safety and Operation - 7890: - Qualitative Test - No setpoints associated	Run Count : 1
January 4, 2024 10:46:22 AM	Start	Execution	Inlet Pressure Accuracy - Front SSL: - Pressure Controlled Inlet - S: 25.0 psi - L: <= 1.2 psi	None
January 4, 2024 10:48:52 AM	End	Execution	Inlet Pressure Accuracy - Front SSL: - Pressure Controlled Inlet - S: 25.0 psi - L: <= 1.2 psi	Run Count : 1
January 4, 2024 10:48:54 AM	Start	Execution	GC Oven Temperature Accuracy - 7890: - Temperature : Oven - S: 230.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	None
January 4, 2024 10:51:05 AM	Audit	Data	GC Oven Temperature Accuracy - 7890: - Temperature : Oven - S: 230.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	Manual Data Entry
January 4, 2024 10:51:08 AM	End	Execution	GC Oven Temperature Accuracy - 7890: - Temperature : Oven - S: 230.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	Run Count : 1
January 4, 2024 10:51:43 AM	Start	Execution	GC Oven Temperature Accuracy - 7890: - Temperature : Oven - S: 100.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	None
January 4, 2024 10:58:45 AM	Audit	Data	GC Oven Temperature Accuracy - 7890: - Temperature : Oven - S: 100.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	Manual Data Entry

Page 2 / 7

User Name: eaknarin_puangsoa
Report Generated by Hostname: ASRYGWX074

System Id: RYG_EN0136
Print Date: January 5, 2024 10:53:25 AM

ALS_OQ_RYG_EN0136 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
January 4, 2024 10:58:46 AM	End	Execution	GC Oven Temperature Accuracy - 7890: - Temperature : Oven - S: 100.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	Run Count : 1
January 4, 2024 10:58:59 AM	Start	Execution	GC Oven Temperature Stability - 7890: - Temperature : Oven - S: 100.0°C - L: <= 0.5°C	None
January 4, 2024 11:23:26 AM	Audit	Data	GC Oven Temperature Stability - 7890: - Temperature : Oven - S: 100.0°C - L: <= 0.5°C	Manual Data Entry
January 4, 2024 11:23:29 AM	End	Execution	GC Oven Temperature Stability - 7890: - Temperature : Oven - S: 100.0°C - L: <= 0.5°C	Run Count : 1
January 4, 2024 11:23:35 AM	Start	Execution	Log Amp - 5977B SQ: - Source: EI - Extractor	None
January 4, 2024 11:43:23 AM	End	Execution	Log Amp - 5977B SQ: - Source: EI - Extractor	Run Count : 1
January 4, 2024 11:43:26 AM	Start	Execution	RFPA - 5977B SQ: - Source: EI - Extractor	None
January 4, 2024 11:53:23 AM	End	Execution	RFPA - 5977B SQ: - Source: EI - Extractor	Run Count : 1
January 4, 2024 11:53:28 AM	Start	Execution	Tune EI - 5977B SQ: - Source: - EI - Extractor Filament 1 (Qualitative - No setpoints associated)	None
January 4, 2024 1:37:26 PM	End	Execution	Tune EI - 5977B SQ: - Source: - EI - Extractor Filament 1 (Qualitative - No setpoints associated)	Run Count : 1
January 4, 2024 1:37:29 PM	Start	Execution	Tune EI - 5977B SQ: - Source: - EI - Extractor Filament 2 (Qualitative - No setpoints associated)	None

Page 3 / 7

User Name: eaknarin_puangsoa

System Id: RYG_EN0136

Report Generated by Hostname: ASRYGWX074

Print Date: January 5, 2024 10:53:25 AM

ALS_OQ_RYG_EN0136 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
January 4, 2024 1:48:59 PM	End	Execution	Tune EI - 5977B SQ: - Source: - Run Count : 1 EI - Extractor Filament 2 (Qualitative - No setpoints associated)	
January 4, 2024 1:49:02 PM	Start	Execution	Scouting Run - Manual Injection, Front SSL, SQ: - Source: - EI - Extractor- Part of GCMS System Preparation	None
January 4, 2024 2:20:35 PM	Audit	AceClosed	Session	None
January 5, 2024 8:28:16 AM	Audit	AceRestarted	Session	None
January 5, 2024 8:28:18 AM	Audit	SessionReloaded	Session	None
January 5, 2024 8:28:29 AM	Start	Qualification	Session	OQ
January 5, 2024 8:28:29 AM	Start	Execution	Scouting Run - Manual Injection, Front SSL, SQ: - Source: - EI - Extractor- Part of GCMS System Preparation	None
January 5, 2024 9:21:29 AM	Audit	Data	Scouting Run - Manual Injection, Front SSL, SQ: - Source: - EI - Extractor- Part of GCMS System Preparation	Data files Path : D:\OQ2024\scout1.D
January 5, 2024 9:21:53 AM	End	Execution	Scouting Run - Manual Injection, Front SSL, SQ: - Source: - EI - Extractor- Part of GCMS System Preparation	Run Count : 1
January 5, 2024 9:21:58 AM	Start	Execution	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 1 - L: >= 1200	None

Page 4 / 7

User Name: eaknarin_puangsopa

System Id: RYG_EN0136

Report Generated by Hostname: ASRYGWX074

Print Date: January 5, 2024 10:53:25 AM

ALS_OQ_RYG_EN0136 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
January 5, 2024 9:25:39 AM	End	Qualification	Session	OQ
January 5, 2024 9:25:39 AM	Start	Reporting	Session	None
January 5, 2024 9:27:46 AM	End	Reporting	Session	None
January 5, 2024 9:27:46 AM	Start	Qualification	Session	OQ
January 5, 2024 9:27:46 AM	Start	Execution	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 1 - L: >= 1200	None
January 5, 2024 9:33:18 AM	Audit	Data	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 1 - L: >= 1200	Data files Path : D:\OQ2024\SN_F1.D
January 5, 2024 9:45:22 AM	End	Execution	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 1 - L: >= 1200	Run Count : 1
January 5, 2024 9:45:32 AM	Start	Execution	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 2 - L: >= 1200	None
January 5, 2024 9:56:15 AM	Audit	Data	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 2 - L: >= 1200	Data files Path : D:\OQ2024\SN_F2.D
January 5, 2024 10:00:19 AM	End	Execution	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 2 - L: >= 1200	Run Count : 1

Page 5 / 7

User Name: eaknarin_puangsoa

System Id: RYG_EN0136

Report Generated by Hostname: ASRYGWX074

Print Date: January 5, 2024 10:53:25 AM

ALS_OQ_RYG_EN0136 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
January 5, 2024 10:03:53 AM	Audit	TestUnlocked	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 2 - L: >= 1200	Deviation filed for Run Count : 1
January 5, 2024 10:03:53 AM	Start	Execution	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 2 - L: >= 1200	None
January 5, 2024 10:13:48 AM	Audit	Data	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 2 - L: >= 1200	Data files Path : D:\OQ2024\SN_F02.D
January 5, 2024 10:17:58 AM	End	Execution	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 2 - L: >= 1200	Run Count : 2
January 5, 2024 10:22:04 AM	Audit	TestUnlocked	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 2 - L: >= 1200	Deviation filed for Run Count : 2
January 5, 2024 10:22:04 AM	Start	Execution	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 2 - L: >= 1200	None
January 5, 2024 10:22:15 AM	Audit	Data	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 2 - L: >= 1200	Data files Path : D:\OQ2024\SN_F02.D
January 5, 2024 10:25:37 AM	End	Execution	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 2 - L: >= 1200	Run Count : 3

User Name: eaknarin_puangsoa

System Id: RYG_EN0136

Report Generated by Hostname: ASRYGWX074

Print Date: January 5, 2024 10:53:25 AM

ALS_OQ_RYG_EN0136 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
January 5, 2024 10:29:11 AM	Audit	TestUnlocked	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 2 - L: >= 1200	Deviation filed for Run Count : 3
January 5, 2024 10:29:11 AM	Start	Execution	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 2 - L: >= 1200	None
January 5, 2024 10:42:05 AM	Audit	Data	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 2 - L: >= 1200	Data files Path : D:\OQ2024\SN_F002.D
January 5, 2024 10:46:34 AM	End	Execution	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 2 - L: >= 1200	Run Count : 4
January 5, 2024 10:46:41 AM	End	Qualification	Session	OQ
January 5, 2024 10:46:41 AM	Start	Reporting	Session	None
January 5, 2024 10:50:27 AM	Audit	Reporting	Session	Report Generated : Certificate
January 5, 2024 10:51:07 AM	Audit	Reporting	Session	Report Generated : Report
January 5, 2024 10:51:29 AM	Audit	Reporting	Session	Report Generated : Certificate
January 5, 2024 10:52:00 AM	Audit	Reporting	Session	Report Generated : Report

Page 7 / 7



JIRANATEE ASSOCIATES CO.,LTD.

Jiranatee Associates Co.,Ltd.
63/14-15, 67/35-36
Petchkasem 7,7/1, Rd. Watthapra, Bangkokyai,
Bangkok 10600 (Thailand)
Tel: +6608680812
Mobile: +66863999453
E-mail: jnac-calibration@jiranatee.com
Web site: www.jiranatee.com

Accredited calibration laboratory
ISO/IEC 17025:2017
NSC-TISI-TIS 17025
CALIBRATION 0367

Air speed measurement laboratory
Calibration services department.



NSC – TISI – TIS 17025
CALIBRATION 0367

Certificate Number

CWS-004-67

CERTIFICATE OF CALIBRATION

Page 1 of 2 Pages

MEASUREMENT ITEM : Cup anemometer
MANUFACTURER : Novalynx
MODEL/TYPE : Sensor: WS-02F
Data logger: 200-WS-25LB
SERIAL NUMBER : Sensor: WSD-A5244
Data logger: A5244
ID NUMBER : BKK_FS0887
CONDITION AS-RECEIVED : Used item
CUSTOMER : ALS laboratory group (Thailand) Co., Ltd.
104 Phatthanakan 40, Phatthanakan Rd, Khwaeng Suan Luang,
Khet Suan Luang, Bangkok 10250 Thailand.

RECEIVED DATE : 25 Dec 2023
MEASUREMENT DATE : 04 Jan 2024
ISSUE DATE : 05 Jan 2024

ENVIRONMENTAL CONDITIONS:

Ambient condition in the laboratory are as follow:

Temperature : 23.0 ± 3.0 °C
Relative Humidity : 55.0 ± 15.0 %RH
Atmospheric Pressure : 1010 ± 10 hPa

PLACE OF CALIBRATION : Eiffel-type wind tunnel of Jiranatee Associates Co., Ltd.

CALIBRATION CONDITIONS

Wind tunnel cross-section area ¹	900	cm ²
Wind direction frontal area ²	100	cm ²
Diameter of mounting pipe ³	-	mm
Blockage ratio of test object ⁴	0.111	[-]

Preconditioning : 24 hours at ambient conditions.
Measurement Condition : The average values during measurement are (23.8) °C, (52.2) %RH and (1010.8) hPa.

TABULATION OF RESULTS:

The table on next page give the measured values.

Calibrated by:

- ☒ Mr. Sorawit Thachalad
☐ Miss Jittraporn Lertsomphol



Approved signatory:

Mr. Parinya Booncharoen
Calibration Department Manager

Calibration procedure:

The Cup anemometer was calibrated against Standard air velocity transducer model: 8455-12 and pitot tube with precision differential pressure meter model: DPM2500 in an close test-section of Eiffel-type wind tunnel with 900 cm² cross test section area. The WI-CL-007 based on IEC 61400-12-1, Wind energy generation systems – Part 12-1: Power performance measurements of electricity producing wind turbines, March 2017 was used as a calibration guideline.

Traceability:

This certificate provides a traceability of The measurement to recognized the national standards, and to realization of the international system of units (SI) through the NIMT (National Metrology Institute of Thailand) via Certificate number: MW-0001-23 and MW-0055-23

Uncertainty of Measurement:

The reported uncertainty of measurement is based on the standard uncertainty multiplied by a coverage factor $k=2$, Which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty has been determined in accordance with the GUM 'Evaluation of measurement data - Guide to the expression of uncertainty in measurement'

REVIEW BY

APPROVED BY

NEXT CAL. DATE

4/7/25

Remark:

- ¹ Nozzle cross-section area of the wind tunnel
² Projected cross-section area of the tested object include mounting pipe
³ Diameter of mounting pipe
⁴ Ratio ² to ¹

MEASUREMENT RESULTS⁵

The Cup anemometer, Unit Under Calibration (UUC) was exercise at 10 m/s for 5 minutes prior to calibration being performed. The standard air velocity 0.5 m/s to 5 m/s was calculated by a standard air velocity transducer which was installed 50 mm away from wind tunnel nozzle and installed 40 mm away from top of the test section and the standard air velocity 5 m/s to 30 m/s was calculated by a pitot tube with precision differential pressure meter which was installed 50 mm away from wind tunnel nozzle and installed 40 mm away from top of the test section, UUC was mounted on a round vertical tube of the lower plate at center of test section. The calibration was carried out under both rising and falling air velocity in the range of 1 m/s to 16 m/s at calibration interval of 1 m/s. The results of calibration and associated measurement uncertainties are reported in the table below.

v_{std}^6 (m/s)	Temp. wind tunnel (°C)	Temp. room (°C)	v_{uuc}^7 (m/s)	Error (m/s)	$U (k=2)$ (m/s)
1.010	23.80	23.75	0.8	-0.2	0.31
2.097	23.64	23.75	1.9	-0.2	0.31
2.998	23.60	23.75	2.9	-0.1	0.31
4.160	23.64	23.75	4.0	-0.2	0.31
5.06	23.40	23.75	5.1	0.0	0.31
6.00	23.80	23.75	6.1	0.1	0.31
7.03	23.34	23.75	7.0	0.0	0.31
7.98	23.62	23.75	8.0	0.0	0.31
8.96	23.16	23.75	9.1	0.1	0.31
10.03	23.50	23.75	10.2	0.2	0.31
11.04	23.10	23.75	11.2	0.2	0.31
12.01	23.50	23.75	12.2	0.2	0.38
13.04	23.18	23.75	13.3	0.3	0.31
14.02	23.50	23.75	14.4	0.3	0.31
15.03	23.22	23.75	15.4	0.3	0.31
16.03	23.48	23.75	16.3	0.3	0.39

Remark:

⁵ Calibration results only count for the tested circumstances and environmental conditions during which calibration took place

⁶ Velocity of standard

⁷ Velocity of Unit Under Calibration

PHOTO OF CALIBRATION SET-UP

Calibration set-up of the Cup anemometer calibration in the wind tunnel of Jiranatee Associates Co., Ltd. The Cup anemometer shown may differ from the calibrated one. Remark: The proportion of the set- up is not true to scale due to imaging geometry.

End of Certificate of Calibration

JIRANATEE ASSOCIATES CO., LTD.



JIRANATEE ASSOCIATES CO.,LTD.

Jiranatee Associates Co.,Ltd.
63/14-15, 67/35-36
Petchkasem 7,7/1, Rd. Watthapra, Bangkokyai,
Bangkok 10600 (Thailand)
Tel: +6608680812
Mobile: +66863999453
E-mail: jnac-calibration@jiranatee.com
Web site: www.jiranatee.com

Accredited calibration laboratory
ISO/IEC 17025:2017
NSC-TISI-TIS 17025
CALIBRATION 0367

Wind direction measurement laboratory
Calibration services department.



Certificate Number

CWD-004-67

CERTIFICATE OF CALIBRATION

Page 1 of 2 Pages

MEASUREMENT ITEM : Wind Direction Sensor
MANUFACTURER : Novalynx
MODEL/TYPE : Sensor: WS-02F
Data logger: 200-WS-25LB
SERIAL NUMBER : Sensor: WSD-A5244
Data logger: A5244
ID NUMBER : BKK_FS0887
CONDITION AS-RECEIVED : Used item
CUSTOMER : ALS laboratory group (Thailand) Co., Ltd.
104 Phatthanakan 40, Phatthanakan Rd, Khwaeng Suan Luang,
Khet Suan Luang, Bangkok 10250 Thailand.

RECEIVED DATE : 25 Dec 2023
MEASUREMENT DATE : 04 Jan 2024
ISSUE DATE : 05 Jan 2024

ENVIRONMENTAL CONDITIONS:

Ambient condition in the laboratory are as follow:

Temperature : 23.0 ± 3.0 °C
Relative Humidity : 55.0 ± 15.0 %RH
Atmospheric Pressure : 1010 ± 10 hPa

PLACE OF CALIBRATION : Eiffel-type wind tunnel of Jiranatee Associates Co., Ltd.

CALIBRATION CONDITION : Wind tunnel cross-section area¹ 900 cm²
Wind direction frontal area² 129 cm²
Diameter of mounting pipe³ - mm
Blockage ratio of test object⁴ 0.143 [-]

Preconditioning : 24 hours at ambient conditions.
Measurement Condition : The average values during measurement are (23.6)°C, (57.5) %RH and (1011.1) hPa.

TABULATION OF RESULTS:

The table on next page give the measured values.

Calibrated by:

- ☒ Mr. Sorawit Thachalad
☐ Miss Jittraporn Lertsomphol



Approved signatory: _____

Mr. Parinya Booncharoen
Calibration Department Manager

Remark:

- ¹ Nozzle cross-section area of the wind tunnel
² Projected cross-section area of the tested object include mounting pipe
³ Diameter of mounting pipe
⁴ Ratio ² to ¹

MEASUREMENT RESULTS ⁵

The wind direction sensor was calibrated against standard rotary encoder by comparison method. During calibration, the measurement was carried out at 45° intervals in clockwise and counterclockwise directions after offset adjustment has been made. The flow speed of wind tunnel (usually 5 m/s) is kept constant while the sensor is rotated around its vertical axis. The results of calibration and associated measurement uncertainties are reported in the table below.

Air speed m/s	D^6_{std} Degree (°)	D^7_{uuc} Degree (°)	Error Degree (°)	$U (k=2)$ Degree (°)
5.02	45.000	42	-3	0.80
	90.000	87	-3	0.80
	135.000	132	-3	0.80
	180.000	179	-1	0.80
	225.000	226	1	0.80
	270.000	273	3	0.80
	315.000	319	4	0.80
	360.000	359	-1	0.80

Remark:

⁵ Calibration results only count for the tested circumstances and environmental conditions during which calibration took place

⁶ Direction of standard

⁷ Direction of Unit Under Calibration

End of Certificate of Calibration





JIRANATEE ASSOCIATES CO.,LTD.

Jiranatee Associates Co.,Ltd.
63/14-15, 67/35-36
Petchkasem 7,7/1, Rd. Watthapra, Bangkokyai,
Bangkok 10600 (Thailand)
Tel: +6608680812
Mobile: +66863999453
E-mail: jnac-calibration@jiranatee.com
Web site: www.jiranatee.com

Accredited calibration laboratory
ISO/IEC 17025:2017
NSC-TISI-TIS 17025
CALIBRATION 0367

Temperature measurement laboratory
Calibration services department.



CERTIFICATE OF CALIBRATION

Certificate No. : CDT-002-67

Page 1 of 2 Pages

MEASUREMENT ITEM : Data Logger with Temperature sensor
MANUFACTURER : Novalynx
MODEL/TYPE : 200-WS-25LB
SERIAL NUMBER : A5244
ID NUMBER : BKK_FS0887
CONDITION AS-RECEIVED : Used item
CUSTOMER : ALS laboratory group (thailand) Co., Ltd.
104 Phatthanakan 40, Phatthanakan Rd.,
Khwaeng Suan Luang, Khet Suan Luang,
Bangkok 10250 Thailand.

RECEIVED DATE : 25 Dec 2023
MEASUREMENT DATE : 04 Jan 2024
ISSUE DATE : 05 Jan 2024

ENVIRONMENTAL CONDITIONS:

Ambient condition in the laboratory are as follow:

Temperature : 23.0 ± 3.0 °C
Relative Humidity : 55.0 ± 15.0 %RH

NOTED: The certificate is valid only to the item calibrated on date and place of calibration.

TABULATION OF RESULTS:

The table on next page give the measured values.

Calibration procedure:

The temperature calibration was done by In-House calibration method as WI-CL-001 according to comparison method with standard digital temperature indicator and standard temperature probe. The temperature scale use was based on ITS-90.

Traceability:

The measurement results are traceable to the international system of units (SI) through National Institute of Metrology Thailand (NIMT) Certificate number: TT-0038-23, Certificate number: ER-0101-23

Reference Used During Calibration:

1. Standard Temperature Probe
Model: STS-100 A500, Serial No.: 667682-09,
Due date: 28 Mar 2024
2. Digital Temperature Indicator
Model: DTI-1000-A MK II, Serial No.: 671407-00591 Due date: 14 Sep 2024

Uncertainty of Measurement:

The reported uncertainty of measurement is based on the standard uncertainty multiplied by a coverage factor $k=2$, Which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty has been determined in accordance with the GUM 'Evaluation of measurement data - Guide to the expression of uncertainty in measurement'

Calibrated by:

- ☐ Mr. Sorawit Thachalad
☐ Miss Jittraporn Lertsomphol
☒ Miss Ruangrumpai Phoommit



Approved signatory:

Mr. Parinya Booncharoen
Calibration Department Manager

Result of Calibration: ☒ Without Adjustment ☐ With Adjustment

Calibration Range: 20 – 40 °C

Function:

Table 3: This equipment was connected with temperature sensor Model: HMP60 S/N: N0330782.
Dimension: Diameter 12 mm. Length 80 mm.

<u>Immersion Depth</u> (mm)	<u>Standard Reading</u> (°C)	<u>UUC Reading</u> (°C)	<u>Error</u> (°C)	<u>Uncertainty</u> (°C)
70	20.054	19.9	-0.2	0.099
70	25.051	24.8	-0.3	0.099
70	30.042	29.7	-0.3	0.099
70	35.034	34.5	-0.5	0.099
70	40.030	39.4	-0.6	0.099

UUC*: Unit Under Calibration

End of Certificate of Calibration





JIRANATEE ASSOCIATES CO.,LTD.

Jiranatee Associates Co.,Ltd
63/14-15, 67/35-36
Petchkasem 7,7/1, Rd. Watthapra, Bangkokyai,
Bangkok 10600 (Thailand)
Tel: +6608680812
Mobile: +66863999453
E-mail: jnac-calibration@jiranatee.com
Web site: www.jiranatee.com

Accredited calibration laboratory
ISO/IEC 17025:2017
NSC-TISI-TIS 17025
CALIBRATION 0367

Relative humidity measurement laboratory
Calibration services department.

CERTIFICATE OF CALIBRATION

Certificate No. : CRH-003-67

Page 1 of 2 Pages

MEASUREMENT ITEM : Relative humidity with data logger
MANUFACTURER : Novalynx
MODEL/TYPE : 200-WS-25LB
SERIAL NUMBER : A5244
ID NUMBER : BKK_FS0887
CONDITION AS-RECEIVED : Used item
CUSTOMER : ALS laboratory group (Thailand) Co., Ltd.
104 Phatthanakan 40, Phatthanakan Rd, Khwaeng Suan Luang,
Khet Suan Luang, Bangkok 10250 Thailand.

RECEIVED DATE : 25 Dec 2023
MEASUREMENT DATE : 04 Jan 2024
ISSUE DATE : 05 Jan 2024

ENVIRONMENTAL CONDITIONS:

Ambient condition in the laboratory are as follow:

Temperature	: 23.0 ± 3.0	°C
Relative Humidity	: 55.0 ± 15.0	%RH

NOTED: The certificate is valid only to the item calibrated on date and place of calibration.

TABULATION OF RESULTS:

The table on next page give the measured values.

Calibration procedure:

The Relative humidity calibration was done by In-House calibration method as WI-CL-010 according to comparison method with Standard Chilled Mirror hygrometer and standard Humidity generator chamber.

Traceability:

This instrument was calibrated using standard equipment whose accuracy is traceability through the NIMT (National Metrology Institute of Thailand) to the international system of units (SI) via Certificate number: TH-0079-23.

Uncertainty of Measurement:

The reported uncertainty of measurement is based on the standard uncertainty multiplied by a coverage factor $k=2$, Which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty has been determined in accordance with the GUM 'Evaluation of measurement data - Guide to the expression of uncertainty in measurement'

Calibrated by:

- ☐ Mr. Sorawit Thachalad
☒ Miss Jittraporn Lertsomphol
☐ Miss Ruangrumpai Phoommit



Approved signatory:

Mr. Parinya Booncharoen
Calibration Department Manager

Measurement Results:

This equipment was connected with Indoor air quality probe and Displayed (UR) on display. Model: HMP60, Serial number: N0330782.

Result of Calibration: ☒ Without Adjustment ☐ With Adjustment

Calibration Range: 20%RH to 80%RH

Table 1: The results of calibration of relative humidity are reported in table below.

<u>Determined</u> (%RH)	<u>Standard Reading</u> (%RH)	<u>UUC Reading</u> (%RH)	<u>Error</u> (%RH)	<u>Uncertainty</u> (%RH)
20.0	20.04	18.8	-1.3	0.40
50.0	51.32	49.0	-2.3	1.0
80.0	82.88	79.2	-3.7	1.6

UUC*: Unit Under Calibration

End of Certificate of Calibration





JIRANATEE ASSOCIATES CO.,LTD.

Jiranatee Associates Co.,Ltd
63/14-15, 67/35-36
Petchkasem 7,7/1, Rd. Watthapra, Bangkokyai,
Bangkok 10600 (Thailand)
Tel: +6608680812
Mobile: +66863999453
E-mail: jnac-calibration@jiranatee.com
Web site: www.jiranatee.com

Accredited calibration laboratory
ISO/IEC 17025:2017
NSC-TISI-TIS 17025
CALIBRATION 0367

Air speed measurement laboratory
Calibration services department.



NSC – TISI – TIS 17025
CALIBRATION 0367

Certificate Number

CWS-005-67

CERTIFICATE OF CALIBRATION

Page 1 of 2 Pages

MEASUREMENT ITEM : Cup anemometer
MANUFACTURER : Novalynx
MODEL/TYPE : Sensor: WS-02F
Data logger: 200-WS-25LB
SERIAL NUMBER : Sensor: WSD-A5261
Data logger: A5261
ID NUMBER : BKK_FS0888
CONDITION AS-RECEIVED : Used item
CUSTOMER : ALS laboratory group (Thailand) Co., Ltd.
104 Phatthanakan 40, Phatthanakan Rd, Khwaeng Suan Luang,
Khet Suan Luang, Bangkok 10250 Thailand.

RECEIVED DATE : 25 Dec 2023
MEASUREMENT DATE : 04 Jan 2024
ISSUE DATE : 05 Jan 2024

ENVIRONMENTAL CONDITIONS:

Ambient condition in the laboratory are as follow:

Temperature : 23.0 ± 3.0 °C
Relative Humidity : 55.0 ± 15.0 %RH
Atmospheric Pressure : 1010 ± 10 hPa

PLACE OF CALIBRATION : Eiffel-type wind tunnel of Jiranatee Associates Co., Ltd.

CALIBRATION CONDITIONS : Wind tunnel cross-section area¹ 900 cm²
Wind direction frontal area² 100 cm²
Diameter of mounting pipe³ - mm
Blockage ratio of test object⁴ 0.111 [-]

Preconditioning : 24 hours at ambient conditions.
Measurement Condition : The average values during measurement are (23.7) °C, (46.6) %RH and (1014.3) hPa.

TABULATION OF RESULTS:

The table on next page give the measured values.

Calibrated by:

☒ Mr. Sorawit Thachalad
☐ Miss Jitraporn Lertsomphol



Approved signatory:

Mr. Parinya Booncharoen
Calibration Department Manager

Remark:

¹ Nozzle cross-section area of the wind tunnel
² Projected cross-section area of the tested object include mounting pipe
³ Diameter of mounting pipe
⁴ Ratio ² to ¹

Calibration procedure:

The Cup anemometer was calibrated against Standard air velocity transducer model: 8455-12 and pitot tube with precision differential pressure meter model: DPM2500 in an close test-section of Eiffel-type wind tunnel with 900 cm² cross test section area. The WI-CL-007 based on IEC 61400-12-1, Wind energy generation systems – Part 12-1: Power performance measurements of electricity producing wind turbines, March 2017 was used as a calibration guideline.

Traceability:

This certificate provides a traceability of The measurement to recognized the national standards, and to realization of the international system of units (SI) through the NIMT (National Metrology Institute of Thailand) via Certificate number: MW-0001-23 and MW-0055-23

Uncertainty of Measurement:

The reported uncertainty of measurement is based on the standard uncertainty multiplied by a coverage factor $k=2$, Which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty has been determined in accordance with the GUM 'Evaluation of measurement data - Guide to the expression of uncertainty in measurement'

REVIEW BY

APPROVED

NEXT CAL DATE

4/7/25

MEASUREMENT RESULTS⁵

The Cup anemometer, Unit Under Calibration (UUC) was exercise at 10 m/s for 5 minutes prior to calibration being performed. The standard air velocity 0.5 m/s to 5 m/s was calculated by a standard air velocity transducer which was installed 50 mm away from wind tunnel nozzle and installed 40 mm away from top of the test section and the standard air velocity 5 m/s to 30 m/s was calculated by a pitot tube with precision differential pressure meter which was installed 50 mm away from wind tunnel nozzle and installed 40 mm away from top of the test section, UUC was mounted on a round vertical tube of the lower plate at center of test section. The calibration was carried out under both rising and falling air velocity in the range of 1 m/s to 16 m/s at calibration interval of 1 m/s. The results of calibration and associated measurement uncertainties are reported in the table below.


V_{std} ⁶ (m/s)	Temp. wind tunnel (°C)	Temp. room (°C)	V_{uuc} ⁷ (m/s)	Error (m/s)	$U (k=2)$ (m/s)
1.016	23.70	23.65	0.9	-0.1	0.31
2.058	23.50	23.65	1.9	-0.2	0.31
2.998	23.78	23.65	2.9	-0.1	0.31
4.168	23.74	23.65	4.0	-0.2	0.31
5.03	23.60	23.65	5.1	0.1	0.31
5.98	23.84	23.65	6.1	0.1	0.31
7.00	23.38	23.65	7.1	0.1	0.31
7.95	23.62	23.65	8.1	0.2	0.31
8.96	23.36	23.65	9.2	0.3	0.31
10.03	23.76	23.65	10.2	0.2	0.31
11.03	23.40	23.65	11.3	0.3	0.31
12.04	23.60	23.65	12.3	0.2	0.31
13.02	23.40	23.65	13.4	0.4	0.31
14.03	23.54	23.65	14.3	0.3	0.31
15.01	23.40	23.65	15.4	0.4	0.31
16.02	23.44	23.65	16.4	0.3	0.33

Remark:


⁵ Calibration results only count for the tested circumstances and environmental conditions during which calibration took place

⁶ Velocity of standard

⁷ Velocity of Unit Under Calibration

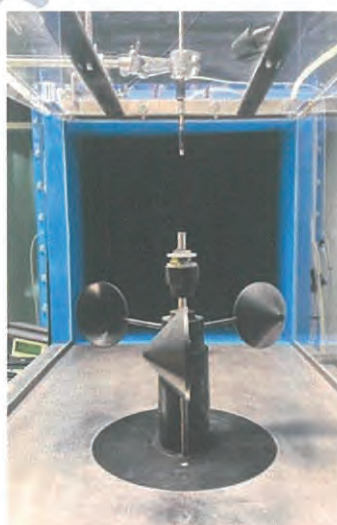PHOTO OF CALIBRATION SET-UP

Calibration set-up of the Cup anemometer calibration in the wind tunnel of Jiranatee Associates Co., Ltd. The Cup anemometer shown may differ from the calibrated one. Remark: The proportion of the set- up is not true to scale due to imaging geometry.

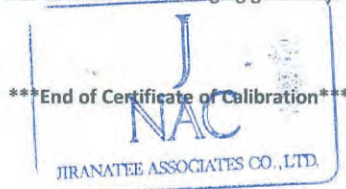



JIRANATEE ASSOCIATES CO.,LTD.

Jiranatee Associates Co.,Ltd
63/14-15, 67/35-36
Petchkasem 7,7/1, Rd. Watthapra, Bangkokyai,
Bangkok 10600 (Thailand)
Tel: +6608680812
Mobile: +66863999453
E-mail: jnac-calibration@jiranatee.com
Web site: www.jiranatee.com

Accredited calibration laboratory
ISO/IEC 17025:2017
NSC-TISI-TIS 17025
CALIBRATION 0367

Wind direction measurement laboratory
Calibration services department.



NSC – TISI – TIS 17025
CALIBRATION 0367

Certificate Number

CWD-005-67

CERTIFICATE OF CALIBRATION

Page 1 of 2 Pages

MEASUREMENT ITEM

MANUFACTURER

MODEL/TYPE

SERIAL NUMBER

ID NUMBER

CONDITION AS-RECEIVED

CUSTOMER

RECEIVED DATE

MEASUREMENT DATE

ISSUE DATE

ENVIRONMENTAL CONDITIONS:

Ambient condition in the laboratory are as follow:

Temperature	: 23.0 ± 3.0	°C
Relative Humidity	: 55.0 ± 15.0	%RH
Atmospheric Pressure	: 1010 ± 10	hPa

PLACE OF CALIBRATION

CALIBRATION CONDITION

Preconditioning

Measurement Condition

TABULATION OF RESULTS:

The table on next page give the measured values.

Calibrated by:

- ☒ Mr. Sorawit Thachalad
☐ Miss Jittraporn Lertsomphol



Approved signatory:

Mr. Parinya Booncharoen
Calibration Department Manager

Remark:

- ¹ Nozzle cross-section area of the wind tunnel
² Projected cross-section area of the tested object include mounting pipe
³ Diameter of mounting pipe
⁴ Ratio ² to ¹

MEASUREMENT RESULTS⁵

The wind direction sensor was calibrated against standard rotary encoder by comparison method. During calibration, the measurement was carried out at 45° intervals in clockwise and counterclockwise directions after offset adjustment has been made. The flow speed of wind tunnel (usually 5 m/s) is kept constant while the sensor is rotated around its vertical axis. The results of calibration and associated measurement uncertainties are reported in the table below.

Air speed m/s	D^s_{std} Degree (°)	D^7_{uuc} Degree (°)	Error Degree (°)	$U (k=2)$ Degree (°)
5.03	45.000	41	-4	0.80
	90.000	87	-3	0.80
	135.001	132	-3	0.80
	180.000	180	0	0.80
	225.000	228	3	0.80
	270.000	274	4	0.80
	315.000	319	4	0.80
	360.000	359	-1	0.80

Remark:

⁵ Calibration results only count for the tested circumstances and environmental conditions during which calibration took place

⁶ Direction of standard

⁷ Direction of Unit Under Calibration

End of Certificate of Calibration





JIRANATEE ASSOCIATES CO.,LTD.

Jiranatee Associates Co.,Ltd.
63/14-15, 67/35-36
Petchkasem 7,7/1, Rd. Watthapra, Bangkokyai,
Bangkok 10600 (Thailand)
Tel: +6608680812
Mobile: +66863999453
E-mail: jnac-calibration@jiranatee.com
Web site: www.jiranatee.com

Accredited calibration laboratory
ISO/IEC 17025:2017
NSC-TISI-TIS 17025
CALIBRATION 0367

Temperature measurement laboratory
Calibration services department.



CERTIFICATE OF CALIBRATION

Certificate No. : CDT-003-67

Page 1 of 2 Pages

MEASUREMENT ITEM : Data Logger with Temperature sensor
MANUFACTURER : Novalynx
MODEL/TYPE : 200-WS-25LB
SERIAL NUMBER : A5261
ID NUMBER : BKK_FS0888
CONDITION AS-RECEIVED : Used item
CUSTOMER : ALS laboratory group (thailand) Co., Ltd.
104 Phatthanakan 40, Phatthanakan Rd.,
Khwaeng Suan Luang, Khet Suan Luang,
Bangkok 10250 Thailand.

RECEIVED DATE : 25 Dec 2023
MEASUREMENT DATE : 04 Jan 2024
ISSUE DATE : 05 Jan 2024

ENVIRONMENTAL CONDITIONS:

Ambient condition in the laboratory are as follow:

Temperature : 23.0 ± 3.0 °C
Relative Humidity : 55.0 ± 15.0 %RH

NOTED: The certificate is valid only to the item calibrated on date and place of calibration.

TABULATION OF RESULTS:

The table on next page give the measured values.

Calibration procedure:

The temperature calibration was done by In-House calibration method as WI-CL-001 according to comparison method with standard digital temperature indicator and standard temperature probe. The temperature scale use was based on ITS-90.

Traceability:

The measurement results are traceable to the international system of units (SI) through National Institute of Metrology Thailand (NIMT) Certificate number: TT-0038-23, Certificate number: ER-0101-23

Reference Used During Calibration:

1. Standard Temperature Probe
Model: STS-100 A500, Serial No.: 667682-09,
Due date: 28 Mar 2024
2. Digital Temperature Indicator
Model: DTI-1000-A MK II, Serial No.: 671407-00591 Due date: 14 Sep 2024

Uncertainty of Measurement:

The reported uncertainty of measurement is based on the standard uncertainty multiplied by a coverage factor $k=2$, Which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty has been determined in accordance with the GUM 'Evaluation of measurement data - Guide to the expression of uncertainty in measurement'

Calibrated by:

- ☐ Mr. Sorawit Thachalad
☐ Miss Jitraporn Lertsomphol
☒ Miss Ruangrumpai Phoommit



Approved signatory:

Mr. Parinya Booncharoen
Calibration Department Manager



JIRANATEE ASSOCIATES CO.,LTD.

Continuation of Certificate of Calibration Number CDT-003-67

Page 2 of 2 Pages

Result of Calibration: ☒ Without Adjustment ☐ With Adjustment

Calibration Range: 20 – 40 °C

Function:

Table 3: This equipment was connected with temperature sensor Model: HMP60 S/N: N0330783.
Dimension: Diameter 12 mm. Length 80 mm.

<u>Immersion Depth</u> (mm)	<u>Standard Reading</u> (°C)	<u>UUC Reading</u> (°C)	<u>Error</u> (°C)	<u>Uncertainty</u> (°C)
70	20.054	19.8	-0.3	0.099
70	25.051	24.6	-0.5	0.099
70	30.043	29.5	-0.5	0.099
70	35.035	34.4	-0.6	0.099
70	40.030	39.3	-0.7	0.099

UUC*: Unit Under Calibration

End of Certificate of Calibration





JIRANATEE ASSOCIATES CO.,LTD.

Jiranatee Associates Co.,Ltd
63/14-15, 67/35-36
Petchkasem 7,7/1, Rd. Watthapra, Bangkokyai,
Bangkok 10600 (Thailand)
Tel: +6608680812
Mobile: +66863999453
E-mail: jnac-calibration@jiranatee.com
Web site: www.jiranatee.com

Accredited calibration laboratory
ISO/IEC 17025:2017
NSC-TISI-TIS 17025
CALIBRATION 0367

Relative humidity measurement laboratory
Calibration services department.

CERTIFICATE OF CALIBRATION

Certificate No. : CRH-004-67

Page 1 of 2 Pages

MEASUREMENT ITEM : Relative humidity with data logger
MANUFACTURER : Novalynx
MODEL/TYPE : 200-WS-25LB
SERIAL NUMBER : A5261
ID NUMBER : BKK_FS0888
CONDITION AS-RECEIVED : Used item
CUSTOMER : ALS laboratory group (Thailand) Co., Ltd.
104 Phatthanakan 40, Phatthanakan Rd, Khwaeng Suan Luang,
Khet Suan Luang, Bangkok 10250 Thailand.

RECEIVED DATE : 25 Dec 2023
MEASUREMENT DATE : 04 Jan 2024
ISSUE DATE : 05 Jan 2024

ENVIRONMENTAL CONDITIONS:

Ambient condition in the laboratory are as follow:

Temperature : 23.0 ± 3.0 °C
Relative Humidity : 55.0 ± 15.0 %RH

NOTED: The certificate is valid only to the item calibrated on date and place of calibration.

TABULATION OF RESULTS:

The table on next page give the measured values.

Calibration procedure:

The Relative humidity calibration was done by In-House calibration method as WI-CL-010 according to comparison method with Standard Chilled Mirror hygrometer and standard Humidity generator chamber.

Traceability:

This instrument was calibrated using standard equipment whose accuracy is traceability through the NIMT (National Metrology Institute of Thailand) to the international system of units (SI) via Certificate number: TH-0079-23.

Uncertainty of Measurement:

The reported uncertainty of measurement is based on the standard uncertainty multiplied by a coverage factor $k=2$, Which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty has been determined in accordance with the GUM 'Evaluation of measurement data - Guide to the expression of uncertainty in measurement'

Calibrated by:

- ☐ Mr. Sorawit Thachalad
☒ Miss Jittraporn Lertsomphol
☐ Miss Ruangrumpai Phoommit



Approved signatory:

Mr. Parinya Booncharoen
Calibration Department Manager



JIRANATEE ASSOCIATES CO.,LTD.

Continuation of Certificate of Calibration Number: CRH-004-67

Page 2 of 2 Pages

Measurement Results:

This equipment was connected with Indoor air quality probe and Displayed (UR) on display. Model: HMP60, Serial number: N0330783.

Result of Calibration: ☒ Without Adjustment ☐ With Adjustment

Calibration Range: 20%RH to 80%RH

Table 1: The results of calibration of relative humidity are reported in table below.

<u>Determined</u> (%RH)	<u>Standard Reading</u> (%RH)	<u>UUC Reading</u> (%RH)	<u>Error</u> (%RH)	<u>Uncertainty</u> (%RH)
20.0	20.04	18.6	-1.5	0.40
50.0	51.31	48.7	-2.6	1.0
80.0	82.85	78.9	-4.0	1.6

UUC*: Unit Under Calibration

End of Certificate of Calibration





JIRANATEE ASSOCIATES CO.,LTD.

Jiranatee Associates Co.,Ltd.
63/14-15, 67/35-36
Petchkasem 7,7/1, Rd. Watthapra, Bangkokyai,
Bangkok 10600 (Thailand)
Tel: +6608680812
Mobile: +66863999453
E-mail: jnac-calibration@jiranatee.com
Web site: www.jiranatee.com

Accredited calibration laboratory
ISO/IEC 17025:2017
NSC-TISI-TIS 17025
CALIBRATION 0367

Air speed measurement laboratory
Calibration services department.



NSC – TISI – TIS 17025
CALIBRATION 0367

Certificate Number

CWS-021-67

CERTIFICATE OF CALIBRATION

Page 1 of 2 Pages

MEASUREMENT ITEM : Cup anemometer
MANUFACTURER : Novalynx
MODEL/TYPE : Sensor: WS-02F
Data logger: 200-WS-25LB
SERIAL NUMBER : Sensor: WSD-A5262
Data logger: A5262
ID NUMBER : BKK_FS0909
CONDITION AS-RECEIVED : Used item
CUSTOMER : ALS laboratory group (Thailand) Co., Ltd.
104 Phatthanakan 40, Phatthanakan Rd, Khwaeng Suan Luang,
Khet Suan Luang, Bangkok 10250 Thailand.

RECEIVED DATE : 10 Jun 2024
MEASUREMENT DATE : 28 Jun 2024
ISSUE DATE : 28 Jun 2024

ENVIRONMENTAL CONDITIONS:

Ambient condition in the laboratory are as follow:

Temperature	: 23.0 ± 3.0	°C
Relative Humidity	: 55.0 ± 15.0	%RH
Atmospheric Pressure	: 1010 ± 10	hPa

PLACE OF CALIBRATION : Eiffel-type wind tunnel of Jiranatee Associates Co., Ltd.

CALIBRATION CONDITIONS	: Wind tunnel cross-section area ¹	900	cm ²
	Wind direction frontal area ²	100	cm ²
	Diameter of mounting pipe ³	-	mm
	Blockage ratio of test object ⁴	0.111	[-]

Preconditioning : 24 hours at ambient conditions.
Measurement Condition : The average values during measurement are (24.2) °C, (43.0) %RH and (1007.6) hPa.

TABULATION OF RESULTS:

The table on next page give the measured values.

Calibrated by:

- ☒ Mr. Sorawit Thachalad
☐ Miss Jitraporn Lertsomphol



Remark:

- ¹ Nozzle cross-section area of the wind tunnel
² Projected cross-section area of the tested object include mounting pipe
³ Diameter of mounting pipe
⁴ Ratio ² to ¹

Calibration procedure:

The Cup anemometer was calibrated against Standard air velocity transducer model: 8455-12 and pitot tube with precision differential pressure meter model: DPM2500 in an close test-section of Eiffel-type wind tunnel with 900 cm² cross test section area. The WI-CL-007 based on IEC 61400-12-1, Wind energy generation systems – Part 12-1: Power performance measurements of electricity producing wind turbines, March 2017 was used as a calibration guideline.

Traceability:

This certificate provides a traceability of The measurement to recognized the national standards, and to realization of the international system of units (SI) through the NIMT (National Metrology Institute of Thailand) via Certificate number: MW-0007-24 and MW-0055-23

Uncertainty of Measurement:

The reported uncertainty of measurement is based on the standard uncertainty multiplied by a coverage factor k=2, Which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty has been determined in accordance with the GUM 'Evaluation of measurement data - Guide to the expression of uncertainty in measurement'

REVIEW BY

APPROVED BY

NEXT CAL. DATE

28/12/25

Approved signatory:

Mr. Parinya Booncharoen
Calibration Department Manager

MEASUREMENT RESULTS ⁵

The Cup anemometer, Unit Under Calibration (UUC) was exercise at 10 m/s for 5 minutes prior to calibration being performed. The standard air velocity 0.5 m/s to 5 m/s was calculated by a standard air velocity transducer which was installed 50 mm away from wind tunnel nozzle and installed 40 mm away from top of the test section and the standard air velocity 5 m/s to 30 m/s was calculated by a pitot tube with precision differential pressure meter which was installed 50 mm away from wind tunnel nozzle and installed 40 mm away from top of the test section, UUC was mounted on a round vertical tube of the lower plate at center of test section. The calibration was carried out under both rising and falling air velocity in the range of 1 m/s to 16 m/s at calibration interval of 1 m/s. The results of calibration and associated measurement uncertainties are reported in the table below.

V_{std} ⁶ (m/s)	Temp. wind tunnel (°C)	Temp. room (°C)	V_{UUC} ⁷ (m/s)	Error (m/s)	U (k=2) (m/s)
1.015	24.10	24.15	0.9	-0.1	0.31
2.038	24.24	24.15	1.8	-0.2	0.31
3.031	24.34	24.15	2.9	-0.1	0.31
4.142	24.28	24.15	3.9	-0.2	0.31
4.98	24.10	24.15	5.0	0.0	0.31
6.04	24.16	24.15	6.1	0.0	0.31
7.05	24.10	24.15	7.1	0.0	0.31
7.98	24.30	24.15	8.1	0.1	0.31
9.05	24.12	24.15	9.1	0.0	0.31
9.98	24.12	24.15	10.2	0.2	0.31
11.01	24.20	24.15	11.1	0.1	0.31
11.99	24.10	24.15	12.2	0.2	0.31
13.01	24.14	24.15	13.2	0.2	0.31
14.06	24.10	24.15	14.2	0.2	0.31
15.06	24.20	24.15	15.2	0.2	0.31
15.99	24.10	24.15	16.3	0.3	0.31

Remark:

⁵ Calibration results only count for the tested circumstances and environmental conditions during which calibration took place

⁶ Velocity of standard

⁷ Velocity of Unit Under Calibration

PHOTO OF CALIBRATION SET-UP

Calibration set-up of the Cup anemometer calibration in the wind tunnel of Jiranatee Associates Co., Ltd. The Cup anemometer shown may differ from the calibrated one. Remark: The proportion of the set- up is not true to scale due to imaging geometry.



Certificate Number

CWD-021-67

CERTIFICATE OF CALIBRATION

Page 1 of 2 Pages

MEASUREMENT ITEM : Wind Direction Sensor
MANUFACTURER : Novalynx
MODEL/TYPE : Sensor: WS-02F
Data logger: 200-WS-25LB
SERIAL NUMBER : Sensor: WSD-A5262
Data logger: A5262
ID NUMBER : BKK_FS0909
CONDITION AS-RECEIVED : Used item
CUSTOMER : ALS laboratory group (Thailand) Co., Ltd.
104 Phatthanakan 40, Phatthanakan Rd, Khwaeng Suan Luang,
Khet Suan Luang, Bangkok 10250 Thailand.

RECEIVED DATE : 10 Jun 2024
MEASUREMENT DATE : 28 Jun 2024
ISSUE DATE : 28 Jun 2024

ENVIRONMENTAL CONDITIONS:

Ambient condition in the laboratory are as follow:

Temperature	: 23.0 ± 3.0	°C
Relative Humidity	: 55.0 ± 15.0	%RH
Atmospheric Pressure	: 1010 ± 10	hPa

PLACE OF CALIBRATION : Eiffel-type wind tunnel of Jiranatee Associates Co., Ltd.

CALIBRATION CONDITION	: Wind tunnel cross-section area ¹	900	cm ²
	Wind direction frontal area ²	129	cm ²
	Diameter of mounting pipe ³	-	mm
	Blockage ratio of test object ⁴	0.143	[-]

Preconditioning : 24 hours at ambient conditions.

Measurement Condition : The average values during measurement are (23.9)°C, (53.3) %RH and (1007.1) hPa.

TABULATION OF RESULTS:

The table on next page give the measured values.

Calibrated by:

- ☒ Mr. Sorawit Thachalad
☐ Miss Jittraporn Lertsomphol



Approved signatory:

Mr. Parinya Booncharoen
Calibration Department Manager

Remark:

- ¹ Nozzle cross-section area of the wind tunnel
² Projected cross-section area of the tested object include mounting pipe
³ Diameter of mounting pipe
⁴ Ratio ² to ¹

MEASUREMENT RESULTS⁵

The wind direction sensor was calibrated against standard rotary encoder by comparison method. During calibration, the measurement was carried out at 45° intervals in clockwise and counterclockwise directions after offset adjustment has been made. The flow speed of wind tunnel (usually 5 m/s) is kept constant while the sensor is rotated around its vertical axis. The results of calibration and associated measurement uncertainties are reported in the table below.

Air speed m/s	D_{std}^6 Degree (°)	D_{unc}^7 Degree (°)	Error Degree (°)	$U (k=2)$ Degree (°)
5.03	45.000	41	-4	0.80
	90.000	87	-3	0.80
	135.000	132	-3	0.80
	180.000	181	1	0.80
	225.000	228	3	0.80
	270.000	275	5	0.80
	315.000	320	5	0.80
	360.000	359	-1	0.80

Remark:

⁵ Calibration results only count for the tested circumstances and environmental conditions during which calibration took place

⁶ Direction of standard

⁷ Direction of Unit Under Calibration

End of Certificate of Calibration





JIRANATEE ASSOCIATES CO.,LTD.

Jiranatee Associates Co.,Ltd
63/14-15, 67/35-36
Petchkasem 7,7/1, Rd. Watthapra, Bangkokyai,
Bangkok 10600 (Thailand)
Tel: +6608680812
Mobile: +66863999453
E-mail: jnac-calibration@jiranatee.com
Web site: www.jiranatee.com

Accredited calibration laboratory
ISO/IEC 17025:2017
NSC-TISI-TIS 17025
CALIBRATION 0367

Temperature measurement laboratory
Calibration services department.



CERTIFICATE OF CALIBRATION

Certificate No. : CDT-107-67

Page 1 of 2 Pages

MEASUREMENT ITEM : Data Logger with Temperature sensor
MANUFACTURER : Novalynx
MODEL/TYPE : 200-WS-25LB
SERIAL NUMBER : A5262
ID NUMBER : BKK_FS0909
CONDITION AS-RECEIVED : Used item
CUSTOMER : ALS laboratory group (thailand) Co., Ltd.
104 Phatthanakan 40, Phatthanakan Rd.,
Khwaeng Suan Luang, Khet Suan Luang,
Bangkok 10250 Thailand.

RECEIVED DATE : 10 Jun 2024
MEASUREMENT DATE : 28 Jun 2024
ISSUE DATE : 28 Jun 2024

ENVIRONMENTAL CONDITIONS:

Ambient condition in the laboratory are as follow:

Temperature : 23.0 ± 3.0 °C
Relative Humidity : 55.0 ± 15.0 %RH

NOTED: The certificate is valid only to the item calibrated on date and place of calibration.

TABULATION OF RESULTS:

The table on next page give the measured values.

Calibration procedure:

The temperature calibration was done by In-House calibration method as WI-CL-001 according to comparison method with standard digital temperature indicator and standard temperature probe. The temperature scale use was based on ITS-90.

Traceability:

The measurement results are traceable to the international system of units (SI) through National Institute of Metrology Thailand (NIMT) Certificate number: TT-0047-24, Certificate number: ER-0101-23

Reference Used During Calibration:

1. Standard Temperature Probe
Model: STS-100 A500, Serial No.: 667682-09,
Due date: 26 Mar 2025
2. Digital Temperature Indicator
Model: DTI-1000-A MK II, Serial No.: 671407-00591 Due date: 14 Sep 2024

Uncertainty of Measurement:

The reported uncertainty of measurement is based on the standard uncertainty multiplied by a coverage factor $k=2$, Which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty has been determined in accordance with the GUM 'Evaluation of measurement data - Guide to the expression of uncertainty in measurement'

Calibrated by:

- ☐ Mr. Sorawit Thachalad
☒ Miss Jittraporn Lertsomphol
☐ Miss Ruangrumpai Phoommit



Approved signatory:

Mr. Parinya Booncharoen
Calibration Department Manager



JIRANATEE ASSOCIATES CO.,LTD.

Continuation of Certificate of Calibration Number CDT-107-67

Page 2 of 2 Pages

Result of Calibration: ☒ Without Adjustment ☐ With Adjustment

Calibration Range: 20 °C to 40 °C

Function:

Table 3: This equipment was connected with temperature sensor Model: HMP60 S/N: N0330785.
Dimension: Diameter 12 mm. Length 80 mm.

<u>Immersion Depth</u> (mm)	<u>Standard Reading</u> (°C)	<u>UUC Reading</u> (°C)	<u>Error</u> (°C)	<u>Uncertainty</u> (°C)
80	20.054	19.6	-0.5	0.099
80	25.051	24.6	-0.5	0.099
80	30.046	29.7	-0.3	0.099
80	35.034	34.5	-0.5	0.099
80	40.042	39.5	-0.5	0.099

UUC*: Unit Under Calibration

End of Certificate of Calibration





JIRANATEE ASSOCIATES CO.,LTD.

Jiranatee Associates Co.,Ltd
63/14-15, 67/35-36
Petchkasem 7,7/1, Rd. Watthapra, Bangkokyai,
Bangkok 10600 (Thailand)
Tel: +6608680812
Mobile: +66863999453
E-mail: jnac-calibration@jiranatee.com
Web site: www.jiranatee.com

Accredited calibration laboratory
ISO/IEC 17025:2017
NSC-TISI-TIS 17025
CALIBRATION 0367

Relative humidity and Air Temperature measurement laboratory
Calibration services department.

CERTIFICATE OF CALIBRATION

Certificate No. : CRT-019-67

Page 1 of 2 Pages

MEASUREMENT ITEM : Relative humidity with data logger
MANUFACTURER : Novalynx
MODEL/TYPE : Data Logger: 200-WS-25LB
Sensor: HMP60
SERIAL NUMBER : Data Logger: A5262
Sensor: N0330785
ID NUMBER : BKK_FS0909
CONDITION AS-RECEIVED : Used item
CUSTOMER : ALS laboratory group (Thailand) Co., Ltd.
104 Phatthanakan 40, Phatthanakan Rd, Khwaeng Suan Luang,
Khet Suan Luang, Bangkok 10250 Thailand.

RECEIVED DATE : 10 Jun 2024
MEASUREMENT DATE : 28 Jun 2024
ISSUE DATE : 28 Jun 2024

ENVIRONMENTAL CONDITIONS:

Ambient condition in the laboratory are as follow:

Temperature : 23.0 ± 3.0 °C
Relative Humidity : 55.0 ± 15.0 %RH

NOTED: The certificate is valid only to the item calibrated on date and place of calibration.

TABULATION OF RESULTS:

The table on next page give the measured values.

Calibration procedure:

The Relative humidity and Air Temperature calibration was done by In-House calibration method as WI-CL-009 and WI-CL-010 according to comparison method with Standard Chilled Mirror hygrometer with Temperature sensor and standard Humidity generator chamber.

Traceability:

The measurements are traceable to the international system of units (SI) through National Institute of Metrology Thailand (NIMT). Certificate number: TH-0079-23 and through Jiranatee Associates Co., Ltd. Certificate number: CDT-001-67.

Uncertainty of Measurement:

The reported uncertainty of measurement is based on the standard uncertainty multiplied by a coverage factor $k=2$, Which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty has been determined in accordance with the GUM 'Evaluation of measurement data - Guide to the expression of uncertainty in measurement'

Calibrated by:

- ☐ Mr. Sorawit Thachalad
☒ Miss Jittraporn Lertsomphol
☐ Miss Ruangrumpai Phoommit



Approved signatory:

Mr. Parinya Booncharoen
Calibration Department Manager



JIRANATEE ASSOCIATES CO.,LTD.

Continuation of Certificate of Calibration Number: CRT-019-67

Page 2 of 2 Pages

Measurement Results:

The results of calibration and associated measurement uncertainties are reported in the table below.

Result of Calibration: ☒ Without Adjustment ☐ With Adjustment

Table 1: The results of calibration of relative humidity at 30 °C are reported in table below.

Calibration Range: 20%RH to 80%RH

<u>Air Temperature</u> (°C)	<u>Standard Reading</u> (%RH)	<u>UUC Reading</u> (%RH)	<u>Error</u> (%RH)	<u>Uncertainty</u> ±(%RH)
29.80	19.61	18.6	-1.0	0.83
29.80	50.49	49.8	-0.6	1.3
29.82	81.68	80.9	-0.8	2.3

UUC*: Unit Under Calibration

End of Certificate of Calibration

