

ภาคผนวก จ
เอกสารสอบเทียบเครื่องมือที่ใช้ในการตรวจวิเคราะห์



ตารางการเทียบเครื่องมือที่ใช้ในการตรวจวัดและวิเคราะห์

Item	Description	Parameter	List of Equipment	Equipment No.	Calibration	Next Calibration
1.	Ambient Air	1,3 Butadiene	Gas Chromatograph/GC 7890	S/N CN10723012	26/06/2024	June 2025
			Mass Spectrometry/MS 5975	S/N US 71236314	26/06/2024	June 2025
		WS & WD	Wind speed and wind direction/Weather Wizard III	S/N WC60908A48	01/08/2024	August 2025
			Wind speed and wind direction/Vantage VUE	S/N Display MT221012035	19/11/2024	November 2025
2.	Water		Wind speed and wind direction/CR200X	S/N 25875	17/10/2024	October 2025
			Wind speed and wind direction/CR200X	S/N 25874	19/09/2024	September 2025
			Wind speed and wind direction/CR200X	S/N 25873	19/09/2024	September 2025
			pH Meter/Horiba F-71G	S/N V3B1F8H3	31/10/2024	October 2025
		TSS, SS	Electronic Balance/XP 205 DR	S/N 1129273885	13/03/2025	March 2026
		DO	DO Meter/HORIBA	S/N D75J0012	10/01/2025	January 2026
		BOD	BOD Incubator/Model i250	S/N 0408-0115-0008	12/03/2025	March 2026
		Oil & Grease	Electronic Balance/XP 205 DR	S/N 1129273885	13/03/2025	March 2026
		NH ₃ -Nitrogen	Spectrophotometer/Blue Star A	S/N 1606UV1507	09/04/2024	January 2026
		Pb	ICP394/PerkinElmer/OPTIMA8000	S/N 078N1310024C	21/03/2025	September 2025
3.	Sound Level	Leq 24 hr	ICP394/PerkinElmer/OPTIMA8000	S/N 078N1310024C	21/03/2025	September 2025
			Sound Calibrator Tenmars/TM-100	S/N 181203570	28/03/2025	March 2026
4.	Working Air	Ethylene Dichloride	Sound Level Meter/ACO 6236	S/N 222038	08/04/2025	April 2026
			Personal Air Sampler/Gilan	S/N 20180806018	21/04/2025	May 2025
			Personal Air Sampler/Gilan	S/N 20180806027	21/04/2025	May 2025
			Personal Air Sampler/Gilan	S/N 20180802087	16/05/2025	June 2025
			Personal Air Sampler/Gilan	S/N 20180806018	16/05/2025	June 2025
			Gas Chromatograph/GC7890B	S/N CN16343040	25/09/2024	September 2025

ตารางการเทียบเครื่องมือที่ใช้ในการตรวจวัดและวิเคราะห์ (ต่อ)

Item	Description	Parameter	List of Equipment	Equipment No.	Calibration	Next Calibration
4.	Working Air (Cont.)	Vinyl Chloride	Personal Air Sampler/Gilian	S/N 20151002115	31/03/2025	April 2025
			Personal Air Sampler/Gilian	S/N 20180803005	31/03/2025	April 2025
			Personal Air Sampler/Gilian	S/N 20180802087	13/05/2025	June 2025
			Personal Air Sampler/Gilian	S/N 20180806018	13/05/2025	June 2025
			Gas Chromatograph/GC78908	S/N CN16343040	25/09/2024	September 2025
			Personal Air Sampler/Gilian	S/N 20151003042	19/02/2025	March 2025
			Personal Air Sampler/Gilian	S/N 20151102097	19/02/2025	March 2025
			Personal Air Sampler/Gilian	S/N 20151003044	19/02/2025	March 2025
			Personal Air Sampler/Gilian	S/N 20151003009	19/02/2025	March 2025
			Personal Air Sampler/Gilian	S/N 20151003041	19/02/2025	March 2025
		1,3 Butadiene	Personal Air Sampler/Gilian	S/N 20151102080	19/02/2025	March 2025
			Personal Air Sampler/Gilian	S/N 20151003042	19/02/2025	March 2025
			Personal Air Sampler/Gilian	S/N 20151003043	19/02/2025	March 2025
			Personal Air Sampler/Gilian	S/N 20151102093	05/06/2025	July 2025
			Personal Air Sampler/Gilian	S/N 20151003003	05/06/2025	July 2025
			Personal Air Sampler/Gilian	S/N 20151003020	05/06/2025	July 2025
			Personal Air Sampler/Gilian	S/N 20151002115	05/06/2025	July 2025
			Personal Air Sampler/Gilian	S/N 20151003043	05/06/2025	July 2025
			Personal Air Sampler/Gilian	S/N 20151102097	05/06/2025	July 2025
			Personal Air Sampler/Gilian	S/N 20180802087	13/06/2025	July 2025
			Personal Air Sampler/Gilian	S/N 20151002115	13/06/2025	July 2025
			Gas Chromatograph/GC78908	S/N CN16343040	25/09/2024	September 2025

Agilent CrossLab Start Up Services

Agilent GCMS Preventive Maintenance Checklist

Agilent Preventive Maintenance provides factory recommended service for your analytical instruments to assure reliable operation and the accuracy of your results.

Delivered by highly trained and certified service engineers using genuine Agilent parts and supplies, Agilent Preventive Maintenance provides everything you need to reduce unplanned downtime and keep your systems operating at their peak. This checklist will be completed at the end of the service and provided to you as a record of the preventive maintenance activities.

Service Engineer Comments

If there are any specific points you wish to note as part of performing the service or other items of interest for the customer, please write include them in this box.

Service Completion

Service request number 6007097419 Date service completed 26 Jun 2021
Agilent signature Adirek D. Customer signature IQD
Total number of pages in this document 8

Introduction

Select the appropriate PM to be done and then perform the checklist under that section

- ☐ Interim Preventive Maintenance 6 months
- ☒ Major Preventive Maintenance Yearly

This checklist covers the following model(s):

Type	Model
SQ	5973 Series MSD
SQ	5975 Series MSD
SQ	5977 Series MSD
TQ	7000 Series MS/MS
TQ	7010 Series MS/MS
QTOF	7200 Series QTOF
QTOF	7250 Series QTOF

Customer Information

- Customers should provide all necessary operating supplies upon request of the engineer.
- A customer representative should be available to the engineer while performing the preventive maintenance procedures. Customers are responsible for regular maintenance and are encouraged to observe the service representative.
- Any parts not included in the Parts Lists section of this document are not part of the recommended Preventive Maintenance service nor are they included in the price of this service.
- If a system requires the use of extra or special procedures and/or parts for the maintenance service, then these must be ordered separately and charged as a repair, which may incur additional costs.

Important Customer Web Links

- For more information about *Agilent Technologies services*, please visit our website using the following URL: <http://www.agilent.com/en-us/products/crosslab-instrument-services/service-repair>
- To access *Agilent University*, visit <http://www.agilent.com/crosslab/university/> to learn about training options, which include online, classroom and onsite delivery. A training specialist can work directly with you to help determine your best options.
- A useful *Agilent Resource Center* web page is available, which includes short videos on maintenance, quick lists of consumables for new instruments, and other valuable information. Check out the Resource Page here: <https://www.agilent.com/en-us/agilentresources>
- Need technical support, FAQs, supplies? – visit our *Support Home page* at <http://www.agilent.com/search/support>
- Get answers. Share insights. Build connections:
Join the *Agilent Community* at <https://community.agilent.com/welcome>

Service Engineer's Responsibilities

- Contact the customer and ensure that all necessary supplies are available before the preventive maintenance visit.
- Complete empty fields with the relevant information.
- Complete the relevant checkboxes in the checklist using either a "X" or tick mark "✓".
- Check **"Section not applicable"** check boxes to indicate services/tasks not delivered, as appropriate.
- Complete the Preventive Maintenance services in the most logical order relevant to the individual system service in the order of the tasks listed.
- Complete the **Service Review** section together with the customer.
- Ask the customer to sign the Service Completion section including the customer's and your signature.

Additional Instruction Notes

- Preventive maintenance is a factory recommended procedure designed to reduce the likelihood of electromechanical failures. Failure to perform preventive maintenance may reduce the long-term reliability of certain instruments and systems. **Two preventative maintenances (PMs) per year are recommended, the Major PM Service will be performed annually with an Interim PM performed 6 months after the Major PM.**

System Information

- ☐ Check this box if an instrument configuration report is attached instead of completing the table.

Instrument System Name and ID

MS 5 075 C

Instrument System Site and Location

Lab

List System Component Product Numbers

List the Serial Numbers of each Component

1. G 3 172 A

US 712363 14

2.

3.

4.

5.

6.

7.

8.

Preparation

- ☒ Discuss any specific issues with the customer before starting.
- ☒ Review the instrument logbook for recorded problems and comments.
- ☒ Save instrument control settings before starting the procedure.
- ☒ Perform a general inspection of the system for cleanliness.
- ☒ Check for proper installation of parts, assemblies, sensors etc.
- ☒ Check system for required installation of components and settings as defined by current Service Notes
- ☒ Check for firmware updates and verify with customers if they would like them installed. Firmware update(s) are strongly recommended.

Customer Responsibilities

Customers should ensure that all necessary operating supplies, consumables, and usage-dependent items such as gases, vials, syringes, calibrant solution and solvents required for successful preventive maintenance are available. A customer representative should be available while the preventive maintenance is being performed.

Important notice for customers

The customer should complete the following before the Support Provider arrives on site:

- ☐ Perform an autotune and retain the printed tune report just prior to the start of the PM to verify performance of the equipment.

Note: it is recommended to have the customer run the autotune and tune evaluation prior to the PM and then start the vent cycle so that the instrument will be ready for the service representative.

Definition of the Task/Recommended items within the document

Task		Recommended			
Yes	No	Interim	Major	As needed	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	Yes selected means that the task was done or the part was required.
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	No selected means that the task was not done or the part was not required.
<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	Interim selected means that this task is recommended to be done at 6-month intervals.
<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	Major selected means that this task is recommended to be done yearly; if the customer would like a service to be done at the 6-month interval then the service could be purchased.
<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	As needed selected means that the task was done or the part was used as needed. For example, there could be two types of filters that could be used and this was the one selected.

Preventive Maintenance Procedures

Yes/No				Interim/Major	Description
<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>		Perform general inspection of system for cleanliness
<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>		Discuss any problems the customer is having with the instrument
<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>		Review customer maintenance records and exclude maintenance on recently serviced items
<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>		Review the most recent autotune report. This will give a starting point for evaluating spectral peaks, baseline noise, peak shape, mass assignments and resolution.

		GCMS	
Yes/No	Interim/Major	Description	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	Record Instrument model no. G 3192 A
<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	Record Instrument serial no. US 71236314
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	Record Rough Vacuum
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	Record Manifold Vacuum
<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	Type of Column installed DB - 627

				System Checks
Yes/No	Interim	Major		Description
<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	Verify that calibration peaks were seen prior to starting the PM
<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	Vent the instrument
<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	Inspect vacuum hoses, pump, exhaust tubing, and power cords for excessive wear.
<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	Visually inspect calibrant levels – PFTBA PFDTD (if appl.), IRM (if appl.). Refill if available.
<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	Look for any obvious external damage or problems.
<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	Clean air intake(s). Cosmetic cover(s) may need to be removed.
<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	Verify system line voltage meets instrument specifications: Yes <input checked="" type="checkbox"/> No <input type="checkbox"/>

				Wet Mechanical vacuum pumps
Yes/No	Interim	Major		Description
<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	Check for evidence of oil leakage. Check pump gasket for leakage.
<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	Drain and replace mechanical pump oil.
<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	Replace Oil Mist Filter if applicable.
<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	Discuss with customer the need for more frequent oil changes if the oil is dirty
<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	Don't use mist filters with Chemical Ionization.
<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	Perform anti-suckback valve test. Power on until side plate is held closed, power off and check that side plate holds closed. Visually confirm that no oil returns up vacuum hose.
				Dry Mechanical vacuum pumps - Diaphragm
Yes/No	Interim	Major		Description
<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	Check for evidence of poor vacuum – Turbo power demand, poor manifold vacuum, etc.
<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	Clear air flow paths of dust.
<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	If vacuum is poor, then replace the diaphragm pump.
<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	Perform anti-suckback valve test. Power on until side plate is held closed, power off and check that side plate holds closed.

				Dry Mechanical vacuum pumps - Scroll
Yes/No	Interim	Major		Description
<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	Replace the tips seal on the IDP pump.
<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	Check for evidence of poor vacuum – Turbo power demand, poor manifold vacuum, etc.
<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	Replace the Exhaust Filter if required.
<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	Discuss with customer the need for more frequent changes, if needed.
<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	Inform customer that pump gas ballast should be installed all the time.
<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	Perform anti-suckback valve test. Power on until side plate is held closed, power off and check that side plate holds closed.

				Cleaning System and Filters
Yes/No	Interim	Major		Description
				Fans
<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	Remove dust from fans and vent covers.
<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	Verify fans are functional and that there is enough space around the instrument for proper cooling.
				Source cleaning
<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	Open analyzer and remove the source.
<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	Disassemble, Clean, Re-assemble source.
<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	Re-install source and close analyzer.
				Filters
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	Replace RMSH-2 Helium gas filter – if applicable.
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	Replace RMSN-2 Nitrogen gas filter – if applicable.
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	Replace RMSHY-2 Hydrogen gas filter – if applicable.
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	CP17988 – Gas Clean Carrier Gas Kit for 7890 for Nitrogen or Helium; Bracket, Mount, and Filter – if applicable.
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	CP17974 – Gas Clean Filter Kit GC/MS 1/8"; Mount and Filter – if applicable.
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	CP17973 – Gas Clean Filter; Replacement Filter – if applicable.
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	5190-9071 – Methane Gas Filter – if applicable

Guidance: If gas filter is replaced, write the change date on the filter using a permanent marker.

				System post-check
Yes/No	Interim	Major		Description
<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	Pump system back down. Wait until system stability has been achieved.
<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	Verify system vacuum reading(s) via the gauge controller.
<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	Leak Check
<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	Verify system in manual tune
<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	Compare against previous tune file report(s)
<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	Change to Tune and verify that all temperatures, pressures, and gas flows reach method set points
<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	Check manually that you have calibration peaks.
<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	EI Autotune Performed

Guidance: If the PM Service is performed prior to a qualification service, then use the qualification procedure as a guide for final instrument setup and checkout.

Service Review

- ☒ Attach available reports/printouts of all tests to this documentation.
- ☒ Record the Preventive Maintenance service activity in the customer's records/logbook. Record the PM event in the Smart Alerts logbook, if applicable.
- ☒ Update/reset instrument maintenance counters as appropriate.
- ☒ Affix the PM sticker to the system or instrument logbook based on the customer's request.
- ☒ Complete the Service Engineer Comments section if there are additional comments.
- ☒ Review this service, parts replaced, and test results obtained with the customer.
- ☐ If the instrument firmware was updated, record the details of the change in the Service Engineer's Comment box. Systems in a compliant environment may need additional documentation.

Agilent Test Results Table

Test Description	Expected Test Result	Actual Test Result

Agilent Consumed Parts List Table

☐ Section not applicable

Part Description	Part Number	Product or Model# where used	Quantity consumed

Signature Page

Service Engineer Comments (optional)

If there are any specific points you wish to note as part of performing the installation on either form of interest to the customer, please write in this box.

Service Completion

Service request number 6007047419 Date service completed 26 Jun 2024

Agilent signature Adirek K. Customer signature 100

Total number of pages in this document 11

Parts – As needed as part of the PM

Common MS Filters and Seals – 5973/5975/5977/7000/7010/7200/7250 Series

					Supplies	
Yes/No	Interim	Major	As needed		Description	Part number
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	Helium gas filter – if required	RMSH-2
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	Nitrogen gas filter – if required	RMSN-2
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	Big Universal Trap, 1/8" fittings, Hydrogen, if required	RMSHY-2
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	Gas Clean Carrier Gas Kit for 7890 for Nitrogen or Helium; Bracket, Mount and Filter – if required	CP17988
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	Gas Clean Filter Kit GC/MS 1/8 in (complete replacement kit) – if required	CP17974
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	Gas Clean GS/MS Filter – if required	CP17973
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	Chemical Ionization Gas Purifier (CI systems) – if required	5190-9071
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	Agilent AVF Platinum, 1 quart	5191-5851

Gas filters need to be changed only if required

MS Maintenance Supplies for 5973/5975/5977 Series

					Supplies	
Yes/No	Interim	Major	As needed		Description	Part number
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	Diffusion pump fluid (Diffusion Pump Models)	6040-0809 Qty 2
<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	IDP-3 Tip Seal Replacement Kit (IDP-3 Dry Pump Models)	G7077-67018
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	IDP-3 Tip Seal Replacement Kit (no tools – CSD P/N)	5190-9561
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	IDP-3 Tip Seal Replacement Kit (no tools – VPD P/N)	IDP3TS
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	Filter element for IDP-3	REPLSLRFILTER2
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	DS42 Oil Mist Eliminator 3/4G & 3/8	SR03706556
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	Exhaust oil mist trap (thread) Edwards/Pfeiffer	G1099-80039

MS Maintenance Supplies for 7000/7010 Series

					Supplies	
Yes/No	Interim	Major	As needed		Description	Part number
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	Nitrogen gas filter	RMSN-2
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	IDP-10 Tip Seal Replacement Kit (IDP-10 Dry Scroll Pump Models)	G7004-67023
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	IDP-10 Tip Seal Replacement Kit (no tools – VPD P/N)	X3807-67000
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	Oil Mist Filter RV5	G6600-80043
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	Filter element for the IDP-10	REPLSLRFILTER1

MS Maintenance Supplies for 7200/7250 Series

					Supplies	
Yes/No	Interim	Major	As needed		Description	Part number
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	Nitrogen gas filter – if required	RMSN-2
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	RIS Probe Maintenance Kit (7200 Series only)	G7005-60170
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	DS202 Oil Mist Eliminator	SR03706800
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	IDP-15 Tip Seal Replacement Kit (IDP-15 Dry Pump Models)	5190-9613
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	IDP-15 Tip Seal Replacement Kit (no tools – VPD P/N)	X3815-67000
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	Filter element, for SH-110/SH-112/IDP-15 exhaust silencer	REPLSLRFILTER
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	DS 3/8 MAG. PLUG AND GASKET	SR03701824

MS Maintenance Supplies for JetClean

					Supplies	
Yes/No	Interim	Major	As needed		Description	Part number

<input type="checkbox"/> <input checked="" type="checkbox"/> <input type="checkbox"/> <input checked="" type="checkbox"/> <input checked="" type="checkbox"/>	Big Universal Trap, 1/8" fittings, Hydrogen, if required	RMSHY-2
---	--	---------

Consumable Parts Reference – Purchasable by customer, not included as part of PM

Common MSD Maintenance Supplies 5973/5975/5977/7000/7010/7200/7250 Series

					Common Recommended Consumables Parts	
Yes/No	Interim	Major	As needed		Description	Part number
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	El High Temperature Filaments	G7005-60061 Qty 2
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	HES El Filaments	G7002-60001
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	LE-El Filaments	G3850-60021
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	CI High Temperature Filament – all MSDs	G7005-60072
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	PFTBA GCMS Tuning Standard calibrant	05971-60571
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	PFDTD calibrant, 1 mL	8500-8510
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	PFET, IRM calibrant for GC QTOF 0.5 mL	5190-0531

MSD Maintenance Supplies 5973/5975/5977 Series

					Supplies	
Yes/No	Interim	Major	As needed		Description	Part number
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	CI Interface tip seal (tip and spring combo)	G1999-60412
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	CI Interface tip seal (tip only)	G3870-20542
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	CI Interface tip seal spring (spring only)	G1999-20023
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	Repeller insulator	G1099-20133 Qty 2
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	Lens insulator/holder (HES)	G7002-20074
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	Ring heater/sensor assembly (HES)	G7002-60043
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	Ceramic insulator for Extractor (HES)	G7002-20064
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	Transfer-Line Tip Cap, Threaded	G3870-20547
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	Transfer-Line Tip Base, Threaded	G3870-20548

MS Maintenance Supplies for 7000/7010 Series

					Supplies	
Yes/No	Interim	Major	As needed		Description	Part number
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	CI Interface tip seal - 7000	G1999-60412
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	CI Interface tip seal - 7010	G7002-60412
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	CI Interface tip seal (tip only)	G3870-20542
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	CI Interface tip seal spring (spring only)	G1999-20023
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	Repeller insulator - 7000	G1099-20133 Qty 2
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	Lens insulator/holder (HES)	G7002-20074
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	Ring heater/sensor assembly (HES)	G7002-60043
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	Ceramic insulator for Extractor (HES)	G7002-20064
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	Transfer-Line Tip Cap, Threaded	G3870-20547
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	Transfer-Line Tip Base, Threaded	G3870-20548

MS Maintenance Supplies for 7200 Series

					Supplies	
Yes/No	Interim	Major	As needed		Description	Part number
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	Extractor Lens Insulator	G7005-20133
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	Ion Focus Insulator	G7005-20442
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	Ring Heater/Sensor Assembly	G7005-60110
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	RIS Xfer Tip	G7005-20542
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	RIS Xfer Tip Spring	G7005-20024

MS Maintenance Supplies for 7250 Series

Supplies					
Yes/No	<input type="checkbox"/>	<input type="checkbox"/>			
Yes/No	Interim	Major	As needed	Description	Part number
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	Lens insulator/holder (HES)	G7002-20074
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	Ring heater/sensor assembly (HES)	G7002-60043
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	Ceramic insulator for Extractor (HES)	G7002-20064
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	Transfer-Line Tip Cap, Threaded	G3870-20547
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	Transfer-Line Tip Base, Threaded	G3870-20548
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	EI Extractor Transfer Tip	G3870-20542
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	CI Tip Compression Spring	G1999-20023

MS Maintenance Supplies for Intuvo 9000 MS Systems

Supplies					
Yes/No	<input type="checkbox"/>	<input type="checkbox"/>			
Yes/No	Interim	Major	As needed	Description	Part number
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	Swaged MS Tail - Packaged	G4590-60009
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	Swaged MS Tail (HES) - Packaged	G4590-60109

Common MS Maintenance Supplies

Parts required					
Yes/No	<input type="checkbox"/>	<input type="checkbox"/>			
Yes/No	Interim	Major	As needed	Description	Part number
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	Abrasive paper, 30 um	5061-5896
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	Alumina powder	393706201
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	Cloths, clean (pkg of 15)	05980-60051
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	Cloths, cleaning (pkg of 300)	9310-4828
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	Cotton swabs (pkg of 100)	5080-5400
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	Gloves, clean, large	8650-0030
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	Gloves, clean, small	8650-0029



THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804, 0-2399-0469

Calibration Certificate

Issued by : Calibration & Test Section : Meteorological Instruments Bureau

Date of Issue 1 August, 2024

Certification No. 284/24

Page : 1 of 2

Object : Wind speed and wind direction

Manufacturer : Davis Instruments Inc.

Type : Weather Wizard III

Serial No. : WC60908A48 ID No. : No.19

Customer : Thai Environmental Technic Limited.
1/6 Soi Ramkhamhaeng 145,
Khwaeng/Khet Saphan Sung, Bangkok 10240.

Calibration Condition : Temperature 25.1 °C Barometric Pressure 1010.9 hPa

NATIONAL STANDARD WIND TUNNEL :

: Micromanometer Theodor Friedrichs FC014 Serial No. 9310119

: HOOK GAGE NO 1425 Pitot Tube Theodor Friedrichs Type 0800.0000 serial 9023

N.I.S.T. Test Reference Number 731/241460 : Standard Velocity at 20 - 30 m/sec

: Ultrasonic Anemometer Model DA-650-3TV (sensor TR-90AH)

Serial Number 110730029 (sensor 120629586)

JAPAN QUALITY ASSURANCE ORGANIZATION : Standard Velocity at 0 - 20 m/sec


Calibrated by :

Mr. Watcharapol Subwat

Mechanical Engineer

Signed :

Mr. Pisood Promsut

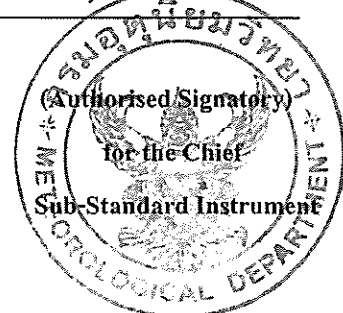



THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804, 0-2399-0469

The Result of Calibration

Certification No. 284/24

1 August, 2024

Page : 2 of 2

Standard Ultrasonic Anemometer m/sec	HOOK GAGE NO. 1425			TESTED ANEMOMETER	
	Pressure inches H ₂ O	Vacumm inches H ₂ O	Velocity m/sec	Velocity m/sec	Correction m/sec
1.00	-	-	-	0.9	0.10
3.02	-	-	-	2.7	0.32
5.00	-	-	-	4.9	0.10
7.00	-	-	-	6.7	0.30
9.02	-	-	-	8.9	0.12
11.01	-	-	-	10.7	0.31
13.01	-	-	-	12.9	0.11
15.01	-	-	-	15.0	0.01
17.02	-	-	-	16.9	0.12
20.02	-	-	-	20.0	0.02

Wind Aloft Plotting Board.	
US.DEPARTMENT OF COMMERCE WEATHER BUREAU	
WIND DIRETION	TESTED WIND DIRECTION
0	0
90	90
180	180
270	270

Calibrated by :

Watcharapol

Mr. Watcharapol Subwat

Mechanical Engineer





THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804, 0-2399-0469

Calibration Certificate

Issued by : Calibration & Test Section : Meteorological Instruments Bureau

Date of Issue 19 November, 2024

Certification No. 416/24

Page : 1 of 2

Object : Wind speed and wind direction

Manufacturer : Davis Instruments Inc.

Type : Vantage VUE Model No. : #6251EU

ID No. : No.33

Serial No. : Display MT221012035 Transmitter MT231004044

Customer : Thai Environmental Technic Limited.

1/6 Soi Ramkhamhaeng 145,

Khwaeng/Khet Saphan Sung, Bangkok 10240.

Calibration Condition : Temperature 25.1 °C Barometric Pressure 1009.6 hPa

NATIONAL STANDARD WIND TUNNEL :

: Micromanometer Theodor Friedrichs FC014 Serial No. 9310119

: HOOK GAGE NO 1425 Pitot Tube Theodor Friedrichs Type 0800.0000 serial 9023

N.I.S.T. Test Reference Number 731/241460 : Standard Velocity at 20 - 30 m/sec

: Ultrasonic Anemometer Model DA-650-3TV (sensor TR-90AH)

Serial Number 110730029 (sensor 120629586)

JAPAN QUALITY ASSURANCE ORGANIZATION : Standard Velocity at 0 - 20 m/sec

Calibrated by :


Watchapol

Mr. Watchapol Subwat

Mechanical Engineer

Signed :

Mr. Pisood Promsut

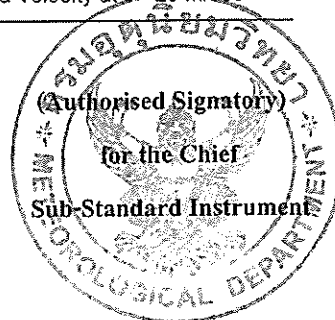



THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804,0-2399-0469

The Result of Calibration

Certification No. 416/24

19 November, 2024

Page : 2 of 2

Standard Ultrasonic Anemometer m/sec	HOOK GAGE NO. 1425			TESTED ANEMOMETER	
	Pressure Inches H2O	Vacumm Inches H2O	Velocity m/sec	Velocity m/sec	Correction m/sec
1.00	-	-	-	0.9	0.10
3.02	-	-	-	2.7	0.32
5.00	-	-	-	4.9	0.10
7.00	-	-	-	6.7	0.30
9.02	-	-	-	9.0	0.02
11.01	-	-	-	10.7	0.31
13.01	-	-	-	13.0	0.01
15.01	-	-	-	15.1	-0.09
17.02	-	-	-	17.0	0.02
20.02	-	-	-	20.1	-0.08


Wind Aloft Plotting Board.	
US.DEPARTMENT OF COMMERCE WEATHER BUREAU	
WIND DIRECTION	TESTED WIND DIRECTION
0	0
90	90
180	180
270	270

Calibrated by :

Watcharapol

Mr. Watcharapol Subwat

Mechanical Engineer

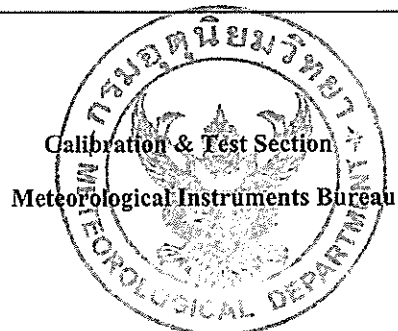



THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804, 0-2399-0469

Calibration Certificate

Issued by : Calibration & Test Section : Meteorological Instruments Bureau

Date of Issue 19 September, 2024

Certification No. 333/24

Page : 1 of 2

Object : Wind speed and wind direction

Manufacturer : Data Logger Campbell Scientific Sensor Young

Type : Data Logger CR200X Sensor 03002

ID No. : No.30

Serial No. : Data Logger 25873 Sensor 014296

Customer : Thai Environmental Technic Limited.
1/6 Soi Ramkhamhaeng 145,
Khwaeng/Khet Saphan Sung, Bangkok 10240.

Calibration Condition : Temperature 25.1 °C Barometric Pressure 1002.5 hPa

NATIONAL STANDARD WIND TUNNEL :

: Micromanometer Theodor Friedrichs FC014 Serial No. 9310119

: HOOK GAGE NO 1425 Pitot Tube Theodor Friedrichs Type 0800.0000 serial 9023

N.I.S.T. Test Reference Number 731/241460 : Standard Velocity at 20 - 30 m/sec

: Ultrasonic Anemometer Model DA-650-3TV (sensor TR-90AH)

Serial Number 110730029 (sensor 120629586)

JAPAN QUALITY ASSURANCE ORGANIZATION : Standard Velocity at 0 - 20 m/sec

Calibrated by :

Wacharapol


Signed :

Pisood Promsut

Mr. Wacharapol Subwat

Mr. Pisood Promsut

Mechanical Engineer

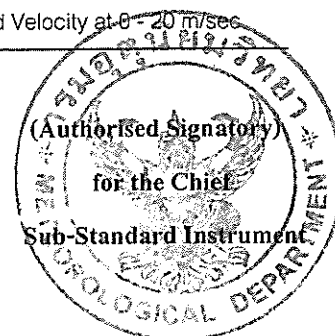



THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804,0-2399-0469

The Result of Calibration

Certification No. 333/24

19 September, 2024

Page : 2 of 2

Standard Ultrasonic Anemometer	HOOK GAGE NO. 1425			TESTED ANEMOMETER	
	Pressure	Vacumm	Velocity	Velocity	Correction
m/sec	inches H2O	inches H2O	m/sec	m/sec	m/sec
1.00	-	-	-	1.06	-0.06
3.02	-	-	-	2.96	0.06
5.00	-	-	-	5.01	-0.01
7.04	-	-	-	7.01	0.03
9.02	-	-	-	9.08	-0.06
11.01	-	-	-	11.00	0.01
13.01	-	-	-	13.05	-0.04
15.01	-	-	-	14.98	0.03
17.02	-	-	-	16.99	0.03
20.02	-	-	-	19.97	0.05

Wind Aloft Plotting Board.	
US.DEPARTMENT OF COMMERCE WEATHER BUREAU	
WIND DIRETION	TESTED WIND DIRECTION
0.00	0
90.00	90.12
180.00	180.08
270.00	270.02

Calibrated by :

Handwritten signature

Mr. Watcharapol Subwat

Mechanical Engineer





THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804, 0-2399-0469

Calibration Certificate

Issued by : Calibration & Test Section : Meteorological Instruments Bureau

Date of Issue 19 September, 2024

Certification No. 334/24

Page : 1 of 2

Object : Wind speed and wind direction

Manufacturer : Data Logger Campbell Scientific Sensor Young

Type : Data Logger CR200X Sensor 03002

ID No. : No.31

Serial No. : Data Logger 25874 Sensor 014294

Customer : Thai Environmental Technic Limited.
1/6 Soi Ramkhamhaeng 145,
Khwaeng/Khet Saphan Sung, Bangkok 10240.

Calibration Condition : Temperature 25.1 °C Barometric Pressure 1002.9 hPa

NATIONAL STANDARD WIND TUNNEL :

: Micromanometer Theodor Friedrichs FC014 Serial No. 9310119


: HOOK GAGE NO 1425 Pitot Tube Theodor Friedrichs Type 0800.0000 serial 9023

N.I.S.T. Test Reference Number 731/241460 : Standard Velocity at 20 - 30 m/sec

: Ultrasonic Anemometer Model DA-650-3TV (sensor TR-90AH)

Serial Number 110730029 (sensor 120629586)


JAPAN QUALITY ASSURANCE ORGANIZATION : Standard Velocity at 0 - 20 m/sec

Calibrated by : 

Mr. Watcharapol Subwat
Mechanical Engineer

Signed :


Mr. Pisood Promsut

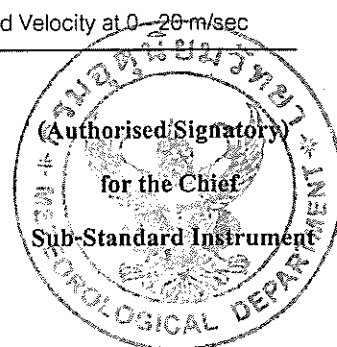



THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804,0-2399-0469

The Result of Calibration

Certification No. 334/24

19 September, 2024

Page : 2 of 2

Standard Ultrasonic Anemometer m/sec	HOOK GAGE NO. 1425			TESTED ANEMOMETER	
	Pressure inches H2O	Vacumm inches H2O	Velocity m/sec	Velocity m/sec	Correction m/sec
1.00	-	-	-	1.06	-0.06
3.02	-	-	-	3.01	0.01
5.00	-	-	-	5.02	-0.02
7.04	-	-	-	7.06	-0.02
9.02	-	-	-	8.99	0.03
11.01	-	-	-	11.05	-0.04
13.01	-	-	-	12.99	0.02
15.01	-	-	-	15.08	-0.07
17.02	-	-	-	17.01	0.01
20.02	-	-	-	20.01	0.01


Wind Aloft Plotting Board.	
US.DEPARTMENT OF COMMERCE WEATHER BUREAU	
WIND DIRETION	TESTED WIND DIRECTION
0.00	0
90.00	90.11
180.00	180.05
270.00	270.06

Calibrated by :

Watcharapol

Mr. Watcharapol Subwat

Mechanical Engineer

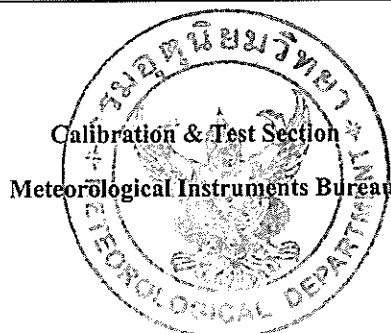



THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804, 0-2399-0469

Calibration Certificate

Issued by : Calibration & Test Section : Meteorological Instruments Bureau

Date of Issue 17 October, 2024

Certification No. 352/24

Page : 1 of 2

Object : Wind speed and wind direction

Manufacturer : Data Logger Campbell Scientific Sensor Young

Type : Data Logger CR200X Sensor 03002

ID No. : No.32

Serial No. : Data Logger 25875 Sensor 014295

Customer : Thai Environmental Technic Limited.
1/6 Soi Ramkhamhaeng 145,
Khwaeng/Khet Saphan Sung, Bangkok 10240.

Calibration Condition : Temperature 25.1 °C Barometric Pressure 1012.0 hPa

NATIONAL STANDARD WIND TUNNEL :

: Micromanometer Theodor Friedrichs FC014 Serial No. 9310119


: HOOK GAGE NO 1425 Pitot Tube Theodor Friedrichs Type 0800.0000 serial 9023

N.I.S.T. Test Reference Number 731/241460 : Standard Velocity at 20 - 30 m/sec

: Ultrasonic Anemometer Model DA-650-3TV (sensor TR-90AH)

Serial Number 110730029 (sensor 120629586)

JAPAN QUALITY ASSURANCE ORGANIZATION : Standard Velocity at 0 - 20 m/sec


Calibrated by : 

Mr. Watcharapol Subwat

Mechanical Engineer

Signed :

Mr. Pisood Promsut

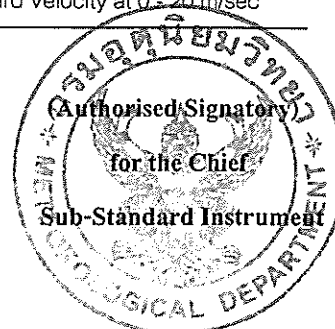



THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804, 0-2399-0469

The Result of Calibration

Certification No. 352/24

17 October, 2024

Page : 2 of 2


Standard Ultrasonic Anemometer m/sec	HOOK GAGE NO. 1425			TESTED ANEMOMETER	
	Pressure inches H ₂ O	Vacumm inches H ₂ O	Velocity m/sec	Velocity m/sec	Correction m/sec
1.00	-	-	-	0.85	0.15
3.02	-	-	-	2.83	0.19
5.00	-	-	-	4.89	0.11
7.04	-	-	-	7.05	-0.01
9.02	-	-	-	9.12	-0.10
11.01	-	-	-	11.42	-0.41
13.01	-	-	-	13.15	-0.14
15.01	-	-	-	15.45	-0.44
17.02	-	-	-	17.12	-0.10
20.02	-	-	-	20.42	-0.40

Wind Aloft Plotting Board.	
US.DEPARTMENT OF COMMERCE WEATHER BUREAU	
WIND DIRETION	TESTED WIND DIRECTION
0.00	0.0
90.00	90.5
180.00	181.1
270.00	270.2

Calibrated by :

Watchapol

Mr. Watchapol Subwat
Mechanical Engineer

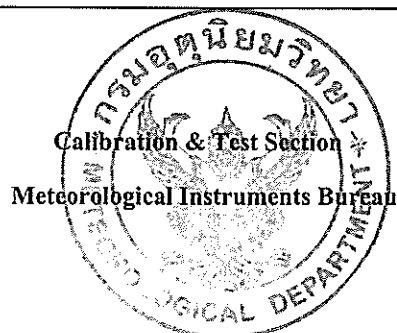



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL.0-2717-3000-29 FAX.0-2719-9484



Certificate of Calibration


Cert.No.: 24CHO573

Page.: 1 of 2

Equipment : pH Meter
Manufacturer : Horiba
Model : F-71G
Serial No. : V3B1F8H3
ID No. : Ins-LAB-025
Condition As-Received: Used Item
Received Date : 30 October 2024
Calibration Date : 31 October 2024
Reference : 2410-0784OC-1
Submitted by : Thai Environmental Technic Limited
1/6 Soi Ramkhamhaeng 145,
Khwaeng/Khet Saphan Sung,
Bangkok 10240

Calibration Place : Laboratory (Thai Environmental Technic Limited)
Ambient Temperature : (26.1 to 25.8) °C (On-Site)
Relative Humidity : (58.6 to 64.2) % (On-Site)
Calibration Procedure : In - house method :
- CP-OCH2 by direct measurement with DC voltage
standard and direct measurement with
certified reference material (CRM)

Calibrated by : Saithip Meangmai

Approved by : 
Approved Signatory

() Unnophol Harachai
(✓) Ponpan Paipim
() Saithip Meangmai

Issue Date : 2 November 2024

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.



Cert.No.: 24CHO573

Page.: 2 of 2

Condition of this calibration result

1. Reference Standard Instrument

<u>Instrument</u>	<u>Serial No.</u>	<u>ID No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
1) Document Process Calibrator	46530031	130RC098	24E3004	12 Sep 2025
2) Digital Thermometer	307901	70RC137	24I973	01 Sep 2025

- This Certification is traceable to SI Through Technology Promotion Association (Thailand - Japan)

2. Certified Reference Materials : The measurement results are traceable to SI through CPA chem Ltd.,
ANSI-ASQ National Accreditation Board, Accredited No. AR-1835

<u>Buffer Solution</u>	<u>Manufacturer</u>	<u>Lot No.</u>	<u>Exp. date</u>
pH 4.008	CPA chem	1034203	27 Sep 2026
pH 6.876	CPA chem	1005301	15 June 2026
pH 9.174	CPA chem	1005302	15 June 2025

3. This certificate is valid only to the item calibrated on date and place of calibration.

Calibration Results**Function : mV Measurement**

Performing standard curve by Document Process Calibrator at pH (4,7,10)

Unit Under Calibration	Nominal Value	Standard Voltage Input	Actual Reading		Uncertainty of Measurement (\pm mV)	Coverage factor <i>k</i>
	pH	mV	mV	pH		
pH Meter S/N.: V3B1F8H3	4.000	177.48	177.5	4.000	0.058	2.00
	6.860	8.28	8.3	6.860	0.058	2.00
	7.000	0.00	0.0	7.000	0.058	2.00
	9.180	-128.97	-128.9	9.180	0.058	2.00
	10.000	-177.48	-177.4	10.000	0.058	2.00

Function : pH Measurement

Performing three buffers standard curve by using buffer nominal pH (4,7,9)

Unit Under Calibration	Standard pH Buffer Solution	Actual pH Reading	Actual mV Reading (mV)	Uncertainty of pH Measurement (\pm)	Coverage factor <i>k</i>
pH Electrode S/N.: 9X2E0223	4.008	4.007	167.0	0.0048	2.00
	6.876	6.855	-0.3	0.0065	2.00
	9.174	9.158	-136.6	0.0096	2.00

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL.0-2717-3000-29 FAX.0-2719-9484



Certificate of Calibration

Cert.No.: 24MM272

Page.: 1 of 3

Equipment : Electronic Balance

Manufacturer : Mettler Toledo

Model : AB204

Serial No. : 1116392227

ID No. : Ins-LAB-033

Submitted by : Thai Environmental Technic Limited
1/6 Soi Ramkhamhaeng 145,
Khwaeng/Khet Saphan Sung,
Bangkok 10240

Location : Balance Room

Received order : 09 April 2024

Calibration Date : 10 April 2024

Ambient Temperature : 15 °C to 40 °C

Relative Humidity : 30 % to 90 %

Calibrated by : Khit Ruttanaprapachai

Approved by :

Kunchit

Approved Signatory

() Ponpan Paipim
() Suwit Imjai
(✓) Kunchit Promprat

Issue Date :

12 April 2024

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.



Equipment : Electronic Balance
Condition As-Received : Used Item
Reference : 2404-0113OC-14

Cert.No.: 24MM272

Page: 2 of 3

Procedure used :-

Calibration were conducted using in-house calibration procedure CP-OB01 based on UKAS LAB 14 according to direct measurement method against standard weight.

Condition of this result of calibration

1. Reference standard instruments:-

<u>Instruments</u>	<u>Model</u>	<u>Serial No.</u>	<u>ID No.</u>	<u>Test report No.</u>	<u>Due date</u>
1) Standard Weight Set (E2)	15884	-	70RC138	MM-0020-23	30 Jan 2025

2. This certificate is valid only to the item calibrated on date and place of calibration.
3. This result of calibration was made on requested at the point specified by customer.
4. This certificate is not certified for any commercial transaction.
5. This certification is traceable to the International System of Unit.

Result of calibration () Without Adjustment (*) After Adjustment by External Calibration

Range capacity : 0 g to 210 g **Resolution** 0.0001 g

Before Adjustment :

<u>Applied Weight</u>	<u>Balance Reading</u>	<u>Correction</u>	<u>Measurement Uncertainty</u>	<u>Coverage Factor</u>
(g)	(g)	(g)	(± mg)	(k)
100	100.0000	0.0000	0.19	2
200	200.0001	-0.0001	0.30	2

After Adjustment :

1. **Determination of the standard deviation of weighing machine** (n = 10)

<u>Applied Weight</u>	<u>Standard Deviation of Reading (g)</u>
(g)	
100	0.00007
200	0.00008



Equipment : Electronic Balance
 Condition As-Received : Used Item
 Reference : 2404-0113OC-14


Cert.No.: 24MM272

Page: 3 of 3

Result of calibration

2. Effect of off center loading

A mass of 100 g was placed to various position on the pan.
 The weighing machine reading error obtained is given in the table

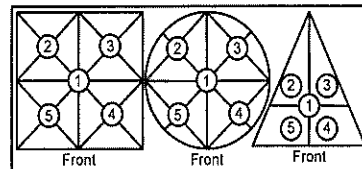

Maximum difference between
 off-center and central loading


Position 1 (g)	Position 2 (g)	Position 3 (g)	Position 4 (g)	Position 5 (g)	(g)
0.0000	+0.0001	0.0000	+0.0001	+0.0003	0.0003

3. Departure from nominal value

<u>Applied Weight</u> (g)	<u>Balance Reading</u> (g)	<u>Correction</u> (g)	<u>Measurement Uncertainty</u> (± mg)	<u>Coverage Factor</u> (k)
Unload	0.0000	0.0000	0.14	2.11
0.01	0.0101	-0.0001	0.14	2.11
0.1	0.1001	-0.0001	0.14	2.11
0.5	0.5002	-0.0002	0.14	2.11
1	1.0002	-0.0002	0.14	2.11
5	5.0000	0.0000	0.14	2.11
10	10.0001	-0.0001	0.14	2.11
25	25.0000	0.0000	0.15	2.07
50	49.9999	+0.0001	0.15	2.06
100	100.0002	-0.0002	0.19	2
200	200.0002	-0.0002	0.30	2

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k , providing a level of confidence of approximately 95 %.

-o0o-



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL.0-2717-3000-29 FAX.0-2719-9484



Certificate of Calibration

Cert. No.: 24TM986

Page : 1 of 3

Equipment : BOD Incubator

Manufacturer : Accuplus

Model : i250-DS

Serial No. : 2059-1017-0029

ID No. : Ins-LAB-047

Submitted by : Thai Environmental Technic Limited
1/6 Soi Ramkhamhaeng 145,
Khwaeng/Khet Saphan Sung,
Bangkok 10240

Location : Laboratory (Thai Environmental Technic Limited)


Received Order : 24 June 2024

Calibration Date : 24 June 2024

Ambient Temperature : (26 ± 10) °C

Relative Humidity : (50 ± 30) %

Calibrated by : Krisda Malee

Approved by : 
Approved Signatory

() Ponpan Paipim
() Suwit Imjai
(✓) Kunchit Promprat

Issue Date : 04 July 2024

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.



Equipment : BOD Incubator
 Condition As-Received : Used Item
 Reference : 2406-0672OC-3

Cert. No.: 24TM986

Page : 2 of 3

Procedure Used :-

Calibration were conducted using calibration procedure CP-OT02 based on TLAS G-20 according to direct measurement method with Data Acquisition which connected with Resistance Temperature Detector (RTD).

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

Instrument	Serial No.	Cert. No.	Traceable	Due Date
1) Data Acquisition	MY57013711	23LM115	TPA	11 Jul 2024

2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certification is traceable to the International System of Unit.


Remark : TPA : Technology Promotion Association (Thailand - Japan)

Result of Calibration :- (*) Without Adjustment

Function of UUC* : Temperature Source

Fresh air setting : Not Available

Environment during calibration		
	Beginning	Finished
Temp. (°C)	24	25
REL.Humid. (%)	53	51
AC Supply (Volt)	220	221

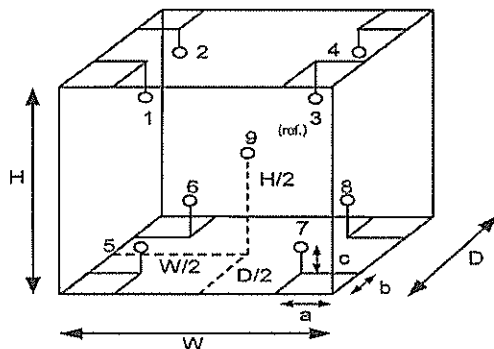

Position :	Ref. Std. ID No.:
1	22-18RTD-2/1
2	18RTD-2/2
3	18RTD-2/3
4	18RTD-2/4
5	18RTD-2/5
6	18RTD-2/6
7	18RTD-2/7
8	18RTD-2/8
9 (ref.)	18RTD-2/9

Probe Installation Details :

a = 10 cm
 b = 10 cm
 c = 10 cm

Dimension of Chamber :

D = 0.48 m
 W = 0.50 m
 H = 1.1 m
 Capacity = 0.26 m³



Equipment : BOD Incubator
Condition As-Received : Used Item
Reference : 2406-0672OC-3
Result of Calibration :- (*) Without Adjustment
Function of UUC* : Temperature Source
Fresh air setting : Not Available

Cert. No.: 24TM986

Page : 3 of 3

Calibration Point (°C)	UUC* Setting (°C)	UUC* Reading (°C)	Temperature stability (± °C)	Temperature uniformity (°C)	Overall Variation (°C)	Coverage Factor <i>k</i>
20.0	20.0	20.0	0.42	0.55	0.99	2

Calibration Point (°C)	Measured Temperature (°C)									Uncertainty (± °C)
	Position									
	1	2	3	4	5	6	7	8	9 (ref.)	
20.0	20.176	20.044	20.228	20.018	20.021	19.995	19.849	19.839	19.863	0.64

Average* : The average of 30 values in each position.

Temperature stability : One-half of the greatest maximum difference of measured temperature at any one sensor.

Temperature uniformity : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.

Overall Variation : The Difference of the maximum and minimum measured temperatures throughout observation.

UUC* : Unit Under Calibration

Note : The reported uncertainty of measurement was included stability and excluded uniformity .

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-



MAINTENANCE REPORT

OPTIMA 8000

Customer : บริษัท เทคนิคสิ่งแวดล้อมไทย Address : จำกัด 1/6 ซอยรามคำแหง 145, แขวงสะพานสูง, เขตสะพานสูง, กรุงเทพฯ 10240 TH User Name: คุณ ธีรพงศ์ โคตะมา Phone: 02-3737799, 081-1303495 E-mail: Ketsarin.Chuayphan@eurofinsasia	Date Tested: March 21, 2025 Recommendation Recertification Period 6 Months Recertification Due: September 22, 2568 Date Last Certified: September 27, 2024 Visit Number: 1 OF 2 TH ONE SOURCE Phone: 081-7316733, 081-1086572 E-mail : thonesource@gmail.com
---	---

CONFIGURATION TESTED	ACCESSORIES/COMPONENT NOT INCLUDED
MODEL OPTIMA 8000 NO772045	SERIAL NUMBER 078S1310024C 1F1380368
TESTED EQUIPMENT IPV Methods	WinLab32 Version 5.5.0 PN:6150T21E4Q1E
TEST STANDARD USED Mixed standard 1/10 Mixed standard 1/100	PE NUMBER N0691579 N9300221
CUSTOMER SUPPLIED 2 % HNO3 10 % HNO3	COMMENTS



MAINTENANCE REPORT

OPTIMA 8000

SERIAL NUMBER 078S1310024C

DATE TESTED

March 21, 2025

1. MECHANICAL CHECKS

- A. Inspect and clean all fans and filters.
- B. Inspect and replace as necessary, all torch components including the RF Flat coil
- C. Inspect all tubing for sign of clacking or leaking.
- D. Adjust water and gas pressure regulator settings.
- E. Inspect and leak check pneumatics drawers.
- F. Clean the exterior of the instrument.

☐ OK☐ OK☐ OK☐ OK☐ OK☐ OK

2. OPTICAL CHECKS

- A. Inspect and clean all optical components.
- B. As required, check and replace all purge filters.
- C. Recheck optical alignment.

☐ OK☐ OK☐ OK

3. COOLING SYSTEM CHECKS

- A. Perform preventive maintenance on chiller.
- B. Flush out water the chiller and replace with coolant mix30plus every twelve months

☐ OK☐ OK

4. PERFORMANCE CHECKS

- A. Torch View Alignment.
- B. Wavelength Calibration.

☐ OK☐ OK



MAINTENANCE REPORT

OPTIMA 8000

SERIAL NUMBER	078S1310024C	DATE TESTED	March 21, 2025
PARAMETER	SPECIFICATION	FINAL VAULE	
Precision			
Zn 213.856	% RSD ≤ 1.0	0.7	
Mg 280.260	% RSD ≤ 1.0	0.37	
Mg 285.207	% RSD ≤ 1.0	0.78	
Ba 455.403	% RSD ≤ 1.0	0.53	
Detection Limits: Axial			
	As 193 nm, 3(sd) ≤ 10.0 ppb	0.9	
	Se 196 nm, 3(sd) ≤ 5.0 ppb	4.73	
	Tl 190 nm, 3(sd) ≤ 10.0 ppb	0.42	
	Pb 220 nm, 3(sd) ≤ 3.0 ppb	0.27	
BEC: Axial	Mn 257 nm, ≤ 30 ppb	1.86	
Detection Limits: Radial			
	As 193 nm, 3(sd) ≤ 60.0 ppb	2.85	
	Zn 213 nm, 3(sd) ≤ 2.0 ppb	0.29	
	Mn 257 nm, 3(sd) ≤ 1.0 ppb	0.03	
	La 379 nm, 3(sd) ≤ 3.0 ppb	0.19	
	Ba 455 nm, 3(sd) ≤ 0.3 ppb	0.01	
	Ba 493 nm, 3(sd) ≤ 0.6 ppb	0.02	
BEC: Radial	Mn 257 nm, ≤ 30 ppb	7.77	
Spectral Resolution: UV			
	As 193 nm, ≤ 0.009	0.00725	
	Ni 231 nm, ≤ 0.011	0.00798	
	Ni 341 nm, ≤ 0.015	0.01218	
Spectral Resolution: VIS			
	Ba 455 nm, ≤ 0.020	0.01540	



MAINTENANCE REPORT

OPTIMA 8000

SERIAL NUMBER 078S1310024C

DATE TESTED

March 21, 2025**Remarks :**

Commissioning follow as commissioning performance sheets.

Calculate MnBEC = $IB * STD \text{ Conc} / IS - IB$, where standard conc = 1000 ug/L

IB = Intensity of blank

IS = Intensity of Standard

Used Mira Mist Nebulizer

This is to certify that the above tests have been performed and the configuration tested



meets



does not meet

This certificate does not modify PerkinElmer's standard terms and condition of sale, including warranty terms.

Service Department TH One Source Co., Ltd.

Krungchai T.

(Krungchai Treevichien)

Customer Support Engineer

=====

Analysis Begun

Start Time: 21/3/2568 14:16:06
 Logged In Analyst: TET
 Spectrometer: Optima 8000

Plasma On Time: 21/3/2568 13:46:44
 Technique: ICP Continuous
 Autosampler: S10

Sample Information File:

Batch ID:
 Results Data Set: DLRL_210325
 Results Library: C:\Users\Public\PerkinElmer\ICP\Data\Results\Results.mdb

Method Loaded

Method Name: DLRL-Cal

Method Last Saved: 27/9/2567 10:48:23

IEC File:

MSF File:

Method Description: Calibration for later test

Sequence No.: 1

Autosampler Location:

Sample ID: Calib Blank 1

Date Collected: 21/3/2568 14:16:10

Analyst:

Data Type: Original

Initial Sample Wt:

Initial Sample Vol:

Dilution:

Sample Prep Vol:

Wash Time:

Nebulizer Parameters: Calib Blank 1

Analyte	Back Pressure	Flow
All	335.0 kPa	0.50 L/min

Mean Data: Calib Blank 1

Analyte	Mean Corrected			RSD	Calib	
	Intensity	Std.Dev.	Conc.		Units	
As 193.696	76.3	5.60	7.34%	[0.00]	mg/L	
Zn 213.857	551.0	13.60	2.47%	[0.00]	mg/L	
Mn 257.610	1670.6	109.17	6.54%	[0.00]	mg/L	
La 379.478	313.1	0.51	0.16%	[0.00]	mg/L	
Ba 455.403	1992.9	244.97	12.29%	[0.00]	mg/L	
Ba 493.408	1949.8	288.76	14.81%	[0.00]	mg/L	

Sequence No.: 2

Autosampler Location:

Sample ID: Calib Std 1

Date Collected: 21/3/2568 14:19:46

Analyst:

Data Type: Original

Initial Sample Wt:

Initial Sample Vol:

Dilution:

Sample Prep Vol:

Wash Time:

Nebulizer Parameters: Calib Std 1

Analyte	Back Pressure	Flow
All	335.0 kPa	0.50 L/min

Mean Data: Calib Std 1

Analyte	Mean Corrected			RSD	Calib	
	Intensity	Std.Dev.	Conc.		Units	
As 193.696	13353.1	71.01	0.53%	[5.0]	mg/L	
Zn 213.857	116888.6	435.46	0.37%	[1.0]	mg/L	
Mn 257.610	1097638.0	20726.98	1.89%	[1.0]	mg/L	
La 379.478	249960.5	2065.12	0.83%	[1.0]	mg/L	
Ba 455.403	601998.4	963.17	0.16%	[0.1]	mg/L	
Ba 493.408	452987.3	4060.62	0.90%	[0.1]	mg/L	

Calibration Summary

Analyte	1	Lin, Calc Int	0.0	2671	0.00000	1.000000
As 193.696	1	Lin, Calc Int	0.0	116900	0.00000	1.000000
Zn 213.857	1	Lin, Calc Int	0.0	1098000	0.00000	1.000000
Mn 257.610	1	Lin, Calc Int	0.0	250000	0.00000	1.000000
La 379.478	1	Lin, Calc Int	0.0			

Ba 455.403	1	Lin, Calc Int	0.0	6020000	0.00000	1.000000
Ba 493.408	1	Lin, Calc Int	0.0	4530000	0.00000	1.000000

```

=====
Sequence No.: 3                      Autosampler Location:
Sample ID: blank                     Date Collected: 21/3/2568 14:22:04
Analyst:                             Data Type: Original
Initial Sample Wt:                   Initial Sample Vol:
Dilution:                           Sample Prep Vol:
Wash Time:
=====

```

```

-----
Nebulizer Parameters: blank
Analyte      Back Pressure  Flow
All          337.0 kPa     0.50 L/min
-----

```

Mean Data: blank

Analyte	Mean Corrected		Calib.	Std.Dev.	Sample		RSD
	Intensity	Conc. Units			Conc. Units	Std.Dev.	
As 193.696	518.3	0.2 mg/L	0.07		194.1 g/L	74.12	38.19%
Zn 213.857	1035.9	0.0 mg/L	0.00		8.9 g/L	2.21	24.90%
Mn 257.610	4078.4	0.0 mg/L	0.00		3.7 g/L	1.19	32.05%
La 379.478	285.8	0.0 mg/L	0.00		1.1 g/L	1.41	123.46%
Ba 455.403	-841.2	-0.0 mg/L	0.00		-0.1 g/L	0.02	15.21%
Ba 493.408	-116.6	-0.0 mg/L	0.00		-0.0 g/L	0.01	55.68%

```

=====
Method Loaded
Method Name: DLRL-Check              Method Last Saved: 25/2/2543 11:12:48
IEC File:                           MSF File:
Method Description: As-60,Zn-2, Mn1.0,La-3,Ba455-0.3,Ba493-0.6
=====

```

```

=====
Sequence No.: 4                      Autosampler Location:
Sample ID: DLRL Check                Date Collected: 21/3/2568 14:25:31
Analyst:                             Data Type: Original
Initial Sample Wt:                   Initial Sample Vol:
Dilution:                           Sample Prep Vol:
Wash Time:
=====

```

```

-----
Nebulizer Parameters: DLRL Check
Analyte      Back Pressure  Flow
All          338.0 kPa     0.50 L/min
-----

```

Mean Data: DLRL Check

Analyte	Mean Corrected		Calib.	Std.Dev.	Sample		RSD
	Intensity	Conc. Units			Conc. Units	Std.Dev.	
As 193.696	-43.5	-0.0 mg/L	0.00		-16.3 g/L	2.85	17.47%
Zn 213.857	-185.0	-0.0 mg/L	0.00		-1.6 g/L	0.29	18.18%
Mn 257.610	-1244.8	-0.0 mg/L	0.00		-1.1 g/L	0.03	3.09%
La 379.478	0.4	0.0 mg/L	0.00		0.0 g/L	0.19	>999.9%
Ba 455.403	-123.3	-0.0 mg/L	0.00		-0.0 g/L	0.01	63.51%
Ba 493.408	-406.5	-0.0 mg/L	0.00		-0.1 g/L	0.02	25.69%

Method Loaded
Method Name: MnBEC
IEC File:
Method Description: XL and RL-Spec <or = 30 g/L,Attn:Spec<or= 50 g/L
Method Last Saved: 1/4/2552 13:47:35
MSF File:

Sequence No.: 4
Sample ID: MnBEC 1ppm Mn
Analyst:
Initial Sample Wt:
Dilution:
Wash Time:
Autosampler Location:
Date Collected: 21/3/2568 14:10:32
Data Type: Original
Initial Sample Vol:
Sample Prep Vol:

Nebulizer Parameters: MnBEC 1ppm Mn
Analyte Back Pressure Flow
All 335.0 kPa 0.50 L/min

Mean Data: MnBEC 1ppm Mn

Analyte	Mean Corrected Intensity	Calib. Conc. Units	Std.Dev.	Sample Conc. Units	Std.Dev.	RSD
Mn 257 XN	10930649.6				20667.67	0.19%
Mn 257 RN	1113096.8				83.06	0.01%

Sequence No.: 5
Sample ID: Blank
Analyst:
Initial Sample Wt:
Dilution:
Wash Time:
Autosampler Location:
Date Collected: 21/3/2568 14:12:50
Data Type: Original
Initial Sample Vol:
Sample Prep Vol:

Nebulizer Parameters: Blank
Analyte Back Pressure Flow
All 334.0 kPa 0.50 L/min

Mean Data: Blank

Analyte	Mean Corrected Intensity	Calib. Conc. Units	Std.Dev.	Sample Conc. Units	Std.Dev.	RSD
Mn 257 XN	28985.2				27708.98	11.58%
Mn 257 RN	10247.0				10525.58	14.93%

Resolution

R 14:01:40.010	03/21/2025	ID: Resolution	As 193.696-Res	Rep 1	Res: 0.00725	nm
R 14:01:47.890	03/21/2025	ID: Resolution	As 193.696-Res	Rep 2	Res: 0.00722	nm
R 14:01:54.645	03/21/2025	ID: Resolution	As 193.696-Res	Rep 3	Res: 0.00720	nm
R 14:02:08.420	03/21/2025	ID: Resolution	Ba 455.403-Res	Rep 1	Res: 0.01540	nm
R 14:02:16.469	03/21/2025	ID: Resolution	Ba 455.403-Res	Rep 2	Res: 0.01538	nm
R 14:02:24.410	03/21/2025	ID: Resolution	Ba 455.403-Res	Rep 3	Res: 0.01536	nm
R 14:02:32.083	03/21/2025	ID: Resolution	Ni 231.604-Res	Rep 1	Res: 0.00794	nm
R 14:02:39.277	03/21/2025	ID: Resolution	Ni 231.604-Res	Rep 2	Res: 0.00797	nm
R 14:02:45.423	03/21/2025	ID: Resolution	Ni 231.604-Res	Rep 3	Res: 0.00798	nm
R 14:02:55.782	03/21/2025	ID: Resolution	Ni 341.476-Res	Rep 1	Res: 0.01214	nm
R 14:03:01.100	03/21/2025	ID: Resolution	Ni 341.476-Res	Rep 2	Res: 0.01216	nm
R 14:03:08.355	03/21/2025	ID: Resolution	Ni 341.476-Res	Rep 3	Res: 0.01218	nm

=====
Analysis Begun

Start Time: 21/3/2568 14:35:56
Logged In Analyst: TET
Spectrometer: Optima 8000

Plasma On Time: 21/3/2568 13:46:44
Technique: ICP Continuous
Autosampler: S10

Sample Information File:

Batch ID:
Results Data Set: DLXL_210325
Results Library: C:\Users\Public\PerkinElmer\ICP\Data\Results\Results.mdb

=====
Method Loaded

Method Name: DLXL-Cal

Method Last Saved: 21/3/2568 14:35:51

IEC File:

MSF File:

Method Description: Calibration for later test

=====
Sequence No.: 1

Sample ID: Calib Blank 1

Autosampler Location:

Date Collected: 21/3/2568 14:36:00

Analyst:

Data Type: Original

Initial Sample Wt:

Initial Sample Vol:

Dilution:

Sample Prep Vol:

Wash Time:

Nebulizer Parameters: Calib Blank 1

Analyte	Back Pressure	Flow
All	339.0 kPa	0.50 L/min

Mean Data: Calib Blank 1

Analyte	Mean Corrected		Std.Dev.	RSD	Calib	
	Intensity				Conc.	Units
As 193.696	111.9		5.49	4.90%	[0.00]	g/L
Se 196.026	30.8		13.59	44.07%	[0.00]	g/L
Tl 190.801	-99.6		4.83	4.85%	[0.00]	g/L
Pb 220.353	438.9		17.54	4.00%	[0.00]	g/L

=====
Sequence No.: 2

Sample ID: DL-Standard

Autosampler Location:

Date Collected: 21/3/2568 14:40:17

Analyst:

Data Type: Original

Initial Sample Wt:

Initial Sample Vol:

Dilution:

Sample Prep Vol:

Wash Time:

Nebulizer Parameters: DL-Standard

Analyte	Back Pressure	Flow
All	339.0 kPa	0.50 L/min

Mean Data: DL-Standard

Analyte	Mean Corrected		Std.Dev.	RSD	Calib	
	Intensity				Conc.	Units
As 193.696	18700.2		1314.60	7.03%	[1000]	g/L
Se 196.026	1154.6		50.48	4.37%	[500]	g/L
Tl 190.801	26633.9		116.96	0.44%	[1000]	g/L
Pb 220.353	48025.5		394.04	0.82%	[500]	g/L

Calibration Summary

Analyte	1	Lin, Calc Int	0.0	18.70	0.00000	1.000000
Se 196.026	1	Lin, Calc Int	0.0	2.309	0.00000	1.000000
Tl 190.801	1	Lin, Calc Int	0.0	26.63	0.00000	1.000000
Pb 220.353	1	Lin, Calc Int	0.0	96.05	0.00000	1.000000

=====
Sequence No.: 3

Sample ID: 10% HNO3

Autosampler Location:

Date Collected: 21/3/2568 14:42:26

Analyst: Data Type: Original
Initial Sample Wt: Initial Sample Vol:
Dilution: Sample Prep Vol:
Wash Time:

Nebulizer Parameters: 10% HNO3
Analyte Back Pressure Flow
All 339.0 kPa 0.50 L/min

Mean Data: 10% HNO3

Analyte	Mean Corrected		Calib.		Sample		RSD
	Intensity	Conc. Units	Std.Dev.	Conc. Units	Std.Dev.		
As 193.696	4824.4	300 g/L	129.60	300 g/L	129.60	50.23%	
Se 196.026	134.4	60 g/L	1.80	60 g/L	1.80	3.10%	
Tl 190.801	90.1	3 g/L	0.89	3 g/L	0.89	26.29%	
Pb 220.353	794.3	8 g/L	2.03	8 g/L	2.03	24.53%	

=====
Method Loaded
Method Name: DLXL-Cal Method Last Saved: 21/3/2568 14:35:51
IEC File: MSF File:
Method Description: Calibration for later test
=====

Sequence No.: 4 Autosampler Location:
Sample ID: Calib Blank 1 Date Collected: 21/3/2568 14:46:50
Analyst: Data Type: Original
Initial Sample Wt: Initial Sample Vol:
Dilution: Sample Prep Vol:
Wash Time:

Nebulizer Parameters: Calib Blank 1
Analyte Back Pressure Flow
All 338.0 kPa 0.50 L/min

Mean Data: Calib Blank 1

Analyte	Mean Corrected		Calib	
	Intensity	Std.Dev.	RSD	Conc. Units
As 193.696	101.1	6.51	6.44%	[0.00] g/L
Se 196.026	51.2	1.08	2.10%	[0.00] g/L
Tl 190.801	-117.0	1.30	1.11%	[0.00] g/L
Pb 220.353	515.6	2.24	0.44%	[0.00] g/L

=====
Sequence No.: 5 Autosampler Location:
Sample ID: DL-Standard Date Collected: 21/3/2568 14:49:35
Analyst: Data Type: Original
Initial Sample Wt: Initial Sample Vol:
Dilution: Sample Prep Vol:
Wash Time:

Nebulizer Parameters: DL-Standard
Analyte Back Pressure Flow
All 340.0 kPa 0.50 L/min

Mean Data: DL-Standard

Analyte	Mean Corrected		Calib	
	Intensity	Std.Dev.	RSD	Conc. Units
As 193.696	17134.3	1980.33	11.56%	[1000] g/L
Se 196.026	1110.8	54.75	4.93%	[500] g/L
Tl 190.801	26518.4	156.43	0.59%	[1000] g/L
Pb 220.353	46195.0	1231.41	2.67%	[500] g/L

Calibration Summary

As 193.696 1 Lin, Calc Int 0.0 17.13 0.00000 1.000000

Se 196.026	1	Lin, Calc Int	0.0	2.222	0.00000	1.000000
Tl 190.801	1	Lin, Calc Int	0.0	26.52	0.00000	1.000000
Pb 220.353	1	Lin, Calc Int	0.0	92.39	0.00000	1.000000

```

=====
Sequence No.: 6                      Autosampler Location:
Sample ID: Sample009                Date Collected: 21/3/2568 14:51:29
Analyst:                            Data Type: Original
Initial Sample Wt:                   Initial Sample Vol:
Dilution:                           Sample Prep Vol:
Wash Time:

```

```

-----
Nebulizer Parameters: Sample009
Analyte          Back Pressure      Flow
All              339.0 kPa          0.50 L/min

```

```

-----
Mean Data: Sample009

```

Analyte	Mean Corrected Intensity	Calib. Conc. Units	Std.Dev.	Sample Conc. Units	Std.Dev.	RSD
As 193.696	16308.0	1000 g/L	516.39	1000 g/L	516.39	54.26%
Se 196.026	252.8	100 g/L	33.71	100 g/L	33.71	29.62%
Tl 190.801	239.8	9 g/L	5.02	9 g/L	5.02	55.49%
Pb 220.353	2360.0	30 g/L	8.13	30 g/L	8.13	31.84%

```

=====
Method Loaded
Method Name: DLXL-Check              Method Last Saved: 25/2/2543 10:51:16
IEC File:                           MSF File:
Method Description: Sample Std.Dev As/Tl <=10 g/l ,Se<=-5 g/l ,Pb<=3 g/l

```

```

=====
Sequence No.: 7                      Autosampler Location:
Sample ID: blank                     Date Collected: 21/3/2568 14:55:38
Analyst:                            Data Type: Original
Initial Sample Wt:                   Initial Sample Vol:
Dilution:                           Sample Prep Vol:
Wash Time:

```

```

-----
Nebulizer Parameters: blank
Analyte          Back Pressure      Flow
All              341.0 kPa          0.50 L/min

```

```

-----
Mean Data: blank

```

Analyte	Mean Corrected Intensity	Calib. Conc. Units	Std.Dev.	Sample Conc. Units	Std.Dev.	RSD
As 193.696	-30.1	-2 g/L	0.90	-2 g/L	0.90	51.37%
Se 196.026	-1.1	-0.5 g/L	4.73	-0.5 g/L	4.73	967.75%
Tl 190.801	-1.1	-0.0 g/L	0.42	-0.0 g/L	0.42	979.48%
Pb 220.353	-30.4	-0.3 g/L	0.27	-0.3 g/L	0.27	82.21%

=====
Method Loaded
Method Name: Precison
IEC File:
Method Description: N=10- 1.0% RSD
Method Last Saved: 22/4/2554 10:20:08
MSF File:

=====
Sequence No.: 3
Sample ID: Precision
Analyst:
Initial Sample Wt:
Dilution:
Wash Time:
Autosampler Location:
Date Collected: 21/3/2568 14:04:01
Data Type: Original
Initial Sample Vol:
Sample Prep Vol:

Nebulizer Parameters: Precision
Analyte Back Pressure Flow
All 332.0 kPa 0.50 L/min

Mean Data: Precision

Analyte	Mean Corrected Intensity	Calib. Conc. Units	Std.Dev.	Sample Conc. Units	Std.Dev.	RSD
Zn 206.200	614769.2				4325.76	0.70%
Mg 280.271	3505593.7				12925.49	0.37%
Mg 285.213	235021.6				1839.02	0.78%
Ba 455.403	7343296.8				38612.33	0.53%

=====

=====

Align View XY Axial for analyte Mn 257.610

X-position	Y-position	Intensity
-2.0	15.0	7246380.1
-1.6	15.0	8749288.5
-1.2	15.0	9975888.0
-0.8	15.0	10666593.7
-0.4	15.0	10492495.9
0.0	15.0	9705889.6
0.4	15.0	8929671.3
0.8	15.0	7301039.6
1.2	15.0	5765113.5
1.6	15.0	4449871.9
2.0	15.0	3078672.1
-0.8	10.0	480288.1
-0.8	10.5	713939.2
-0.8	11.0	1279884.5
-0.8	11.5	2458135.3
-0.8	12.0	3851484.4
-0.8	12.5	5388352.0
-0.8	13.0	7124896.4
-0.8	13.5	9153645.7
-0.8	14.0	10246467.4
-0.8	14.5	10783623.9
-0.8	15.0	10803236.1
-0.8	15.5	10013967.2
-0.8	16.0	9037996.9
-0.8	16.5	7531325.8
-0.8	17.0	5609276.4
-0.8	17.5	4221123.3
-0.8	18.0	2953986.3
-0.8	18.5	1843660.9
-0.8	19.0	941095.9
-0.8	19.5	504994.6
-0.8	20.0	221408.2
-1.6	15.0	9268902.0
-1.2	15.0	10098147.0
-0.8	15.0	10629213.6
-0.4	15.0	10528075.8
0.0	15.0	10112987.0
-0.8	13.0	7614807.0
-0.8	13.5	9046084.3
-0.8	14.0	10391096.5
-0.8	14.5	10795800.0
-0.8	15.0	10843088.3
-0.8	15.5	10239869.2
-0.8	16.0	9049883.9
-0.8	16.5	7671109.4
-0.8	17.0	5666617.0

21/3/2568 13:52:20 aligned for analyte Mn 257.610

X viewing position set to -0.8 mm having Peak intensity 10843088.3 for Axial viewing

Y viewing position set to 15.0 mm having Peak intensity 10843088.3 for Axial viewing

=====

Align View X Radial for analyte Mn 257.610

X-position	Y-position	Intensity
-7.0	15.0	20677.7
-6.5	15.0	23939.2
-6.0	15.0	28571.4
-5.5	15.0	36462.3
-5.0	15.0	50913.7
-4.5	15.0	75265.5
-4.0	15.0	106378.1
-3.5	15.0	150006.1
-3.0	15.0	231723.3
-2.5	15.0	402850.4
-2.0	15.0	579076.7
-1.5	15.0	757804.1
-1.0	15.0	922437.5
-0.5	15.0	999617.5
0.0	15.0	1046887.4
0.5	15.0	960157.6
1.0	15.0	805974.3

1.5	15.0	571806.1
2.0	15.0	284353.0
2.5	15.0	52417.2
3.0	15.0	35745.5
3.5	15.0	33557.2
4.0	15.0	43838.7
4.5	15.0	52890.6
5.0	15.0	59418.3
5.5	15.0	57105.9
6.0	15.0	51241.2
6.5	15.0	43337.0
7.0	15.0	33069.0

21/3/2568 13:55:51 aligned for analyte Mn 257.610
X viewing position set to 0.0 mm having Peak intensity 1046887.4 for Radial viewing
=====




TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL.0-2717-3000-29 FAX.0-2719-9484



Certificate of Calibration

Cert.No.: 24CHO573

Page.: 1 of 2

Equipment : pH Meter
Manufacturer : Horiba
Model : F-71G
Serial No. : V3B1F8H3
ID No. : Ins-LAB-025
Condition As-Received: Used Item
Received Date : 30 October 2024
Calibration Date : 31 October 2024
Reference : 2410-0784OC-1
Submitted by : Thai Environmental Technic Limited
1/6 Soi Ramkhamhaeng 145,
Khwaeng/Khet Saphan Sung,
Bangkok 10240
Calibration Place : Laboratory (Thai Environmental Technic Limited)
Ambient Temperature : (26.1 to 25.8) °C (On-Site)
Relative Humidity : (58.6 to 64.2) % (On-Site)
Calibration Procedure : In - house method :
- CP-OCH2 by direct measurement with DC voltage
standard and direct measurement with
certified reference material (CRM)
Calibrated by : Saithip Meangmai
Approved by : 
Approved Signatory
() Unnopphol Harachai
(✓) Ponpan Paipim
() Saithip Meangmai
Issue Date : 2 November 2024

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3: Equipment Calibration and Testing Services.



Cert.No.: 24CHO573

Page.: 2 of 2

Condition of this calibration result

1. Reference Standard Instrument

<u>Instrument</u>	<u>Serial No.</u>	<u>ID No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
1) Document Process Calibrator	46530031	130RC098	24E3004	12 Sep 2025
2) Digital Thermometer	307901	70RC137	24I973	01 Sep 2025

- This Certification is traceable to SI Through Technology Promotion Association (Thailand - Japan)

2. Certified Reference Materials : The measurement results are traceable to SI through CPA chem Ltd.,
ANSI-ASQ National Accreditation Board, Accredited No. AR-1835

<u>Buffer Solution</u>	<u>Manufacturer</u>	<u>Lot No.</u>	<u>Exp. date</u>
pH 4.008	CPA chem	1034203	27 Sep 2026
pH 6.876	CPA chem	1005301	15 June 2026
pH 9.174	CPA chem	1005302	15 June 2025

3. This certificate is valid only to the item calibrated on date and place of calibration.

Calibration Results

Function : mV Measurement

Performing standard curve by Document Process Calibrator at pH (4,7,10)

Unit Under Calibration	Nominal Value	Standard Voltage Input	Actual Reading		Uncertainty of Measurement (\pm mV)	Coverage factor <i>k</i>
	pH	mV	mV	pH		
pH Meter S/N.: V3B1F8H3	4.000	177.48	177.5	4.000	0.058	2.00
	6.860	8.28	8.3	6.860	0.058	2.00
	7.000	0.00	0.0	7.000	0.058	2.00
	9.180	-128.97	-128.9	9.180	0.058	2.00
	10.000	-177.48	-177.4	10.000	0.058	2.00

Function : pH Measurement

Performing three buffers standard curve by using buffer nominal pH (4,7,9)

Unit Under Calibration	Standard pH Buffer Solution	Actual pH Reading	Actual mV Reading (mV)	Uncertainty of pH Measurement (\pm)	Coverage factor <i>k</i>
pH Electrode S/N.: 9X2E0223	4.008	4.007	167.0	0.0048	2.00
	6.876	6.855	-0.3	0.0065	2.00
	9.174	9.158	-136.6	0.0096	2.00

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL.0-2717-3000-29 FAX.0-2719-9484



Certificate of Calibration

Cert.No.: 24MM272

Page.: 1 of 3

Equipment : Electronic Balance

Manufacturer : Mettler Toledo

Model : AB204

Serial No. : 1116392227


ID No. : Ins-LAB-033

Submitted by : Thai Environmental Technic Limited
1/6 Soi Ramkhamhaeng 145,
Khwaeng/Khet Saphan Sung,
Bangkok 10240

Location : Balance Room

Received order : 09 April 2024
Calibration Date : 10 April 2024
Ambient Temperature : 15 °C to 40 °C
Relative Humidity : 30 % to 90 %

Calibrated by : Khit Ruttanaprapachai

Approved by : 
Approved Signatory

() Ponpan Paipim
() Suwit Imjai
(✓) Kunchit Promprat

Issue Date :

12 April 2024

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.



Equipment : Electronic Balance
Condition As-Received : Used Item
Reference : 2404-0113OC-14
Procedure used :-

Cert.No.: 24MM272
Page: 2 of 3

Calibration were conducted using in-house calibration procedure CP-OB01 based on UKAS LAB 14 according to direct measurement method against standard weight.

Condition of this result of calibration

1. Reference standard instruments:-

<u>Instruments</u>	<u>Model</u>	<u>Serial No.</u>	<u>ID No.</u>	<u>Test report No.</u>	<u>Due date</u>
1) Standard Weight Set (E2)	15884	-	70RC138	MM-0020-23	30 Jan 2025
2. This certificate is valid only to the item calibrated on date and place of calibration.					
3. This result of calibration was made on requested at the point specified by customer.					
4. This certificate is not certified for any commercial transaction.					
5. This certification is traceable to the International System of Unit.					

Result of calibration () Without Adjustment (*) After Adjustment by External Calibration

Range capacity : 0 g to 210 g **Resolution** 0.0001 g

Before Adjustment :

<u>Applied Weight</u>	<u>Balance Reading</u>	<u>Correction</u>	<u>Measurement Uncertainty</u>	<u>Coverage Factor</u>
(g)	(g)	(g)	(\pm mg)	(k)
100	100.0000	0.0000	0.19	2
200	200.0001	-0.0001	0.30	2

After Adjustment :

1. **Determination of the standard deviation of weighing machine** (n = 10)

<u>Applied Weight</u>	<u>Standard Deviation of Reading (g)</u>
(g)	
100	0.00007
200	0.00008



Equipment : Electronic Balance
 Condition As-Received : Used Item
 Reference : 2404-0113OC-14


Cert.No.: 24MM272

Page: 3 of 3

Result of calibration

2. Effect of off center loading

A mass of 100 g was placed at various positions on the pan.
 The weighing machine reading error obtained is given in the table

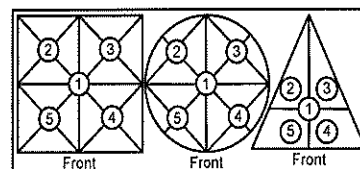

Maximum difference between
 off-center and central loading
 (g)
 0.0003

Position 1 (g)	Position 2 (g)	Position 3 (g)	Position 4 (g)	Position 5 (g)
0.0000	+0.0001	0.0000	+0.0001	+0.0003

3. Departure from nominal value

Applied Weight (g)	Balance Reading (g)	Correction (g)	Measurement Uncertainty (\pm mg)	Coverage Factor (k)
Unload	0.0000	0.0000	0.14	2.11
0.01	0.0101	-0.0001	0.14	2.11
0.1	0.1001	-0.0001	0.14	2.11
0.5	0.5002	-0.0002	0.14	2.11
1	1.0002	-0.0002	0.14	2.11
5	5.0000	0.0000	0.14	2.11
10	10.0001	-0.0001	0.14	2.11
25	25.0000	0.0000	0.15	2.07
50	49.9999	+0.0001	0.15	2.06
100	100.0002	-0.0002	0.19	2
200	200.0002	-0.0002	0.30	2

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k , providing a level of confidence of approximately 95 %.

-o0o-



Certificate of Calibration

Certificate Number : SPR25010086-1

Page : 1 of 3

Customer : Thai Environmental Technic Limited.

1/6 Soi Ramkhamhaeng 145, Khwaeng Saphan Sung, Khet Saphan
Sung, Bangkok 10240, Thailand.

Equipment Name : DO Meter

Manufacturer : Horiba

Model : OM-71G

Serial Number : D75J0012

ID. Number : No.07

Environmental Conditions

Ambient Temperature : $23^{\circ}\text{C} \pm 2^{\circ}\text{C}$

Received Date : 08 Jan 2025

Relative Humidity : $50\% \pm 15\%$

Calibration Date : 10 Jan 2025

Location of Calibration : In-Lab

Recommend Due Date : 10 Jan 2026

Calibration Procedure : In-House Method

Date of Issue : 11 Jan 2025

Method of Calibration


This certifies that the above instrument was calibrated in compliance with the calibration system requirement of ISO/IEC 17025:2017 in accordance with reference procedure. Standards used to perform this calibration are certified by to NIST or equivalent, National metrology institute, Natural physical constants, consensus standards. The result reported herein apply only to the calibration of the item described above as received. Our decision rule is to contact the customer if the item pass and fail calibration when the results include the uncertainties and the customer must determine if the results meets their needs.

The calibration certificate shall not be reproduced except in full, without written approval of SP Metrology System (Thailand).

Calibrated by : Mr.Krittapas Kanchanajittadet

Approved by :

Calibration Officer


(Mr. Prayoon Topart)

Authorized Signatory



Calibration Report

Certificate Number : SPR25010086-1


Page : 2 of 3

Reference Standards

Equipment Name	Model	Serial No.	Certificate No.	Due. Date
Zero Oxygen Solution	HI7040L	Lot S0027-23 _	21C31	21 Mar 2028

Traceability

This certification is traceable to the International System of Unit maintained at :
HANNA - Hanna Instruments (Thailand) Ltd.



Result of Calibration

Certificate Number : SPR25010086-1

Page : 3 of 3

Dissolved Oxygen Permanance Test

Unit : mg/L

Actual Standard	UUC Reading	Error	Uncertainty (±)
0.3	0.51	0.21	0.13
8.3	8.52	0.22	0.13


Note :

The result of calibration was found accurate as show on date and place of calibration only.
This Certificate is not certified for any commercial transaction.

Measurement Uncertainty

The reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor $k = 2.00$, providing a level of confidence approximately 95%.

– End of Certificate –



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL.0-2717-3000-29 FAX.0-2719-9484



Certificate of Calibration

Cert. No.: 24TM702

Page : 1 of 3

Equipment : BOD Incubator

Manufacturer : Accuplus

Model : i250

Serial No. : 0408-0115-0008

ID No. : Ins-LAB-046

Submitted by : Thai Environmental Technic Limited
1/6 Soi Ramkhamhaeng 145,
Khwaeng/Khet Saphan Sung,
Bangkok 10240

Location : Laboratory (Thai Environmental Technic Limited)


Received Order : 09 April 2024

Calibration Date : 09 April 2024

Ambient Temperature : (26 ± 10) °C

Relative Humidity : (50 ± 30) %

Calibrated by : Khit Ruttanaprapachai

Approved by : 
Approved Signatory

() Ponpan Paipim
() Suwit Imjai
(✓) Kunchit Promprat

Issue Date : 26 April 2024

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.



Equipment : BOD Incubator
 Condition As-Received : Used Item
 Reference : 2404-0113OC-11

Cert. No.: 24TM702

Page : 2 of 3

Procedure Used :-

Calibration were conducted using calibration procedure CP-OT02 based on TLAS G-20 according to direct measurement method with Data Acquisition which connected with Resistance Temperature Detector (RTD).

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

Instrument	Serial No.	Cert. No.	Traceable	Due Date
1) Data Acquisition	MY49001451	24LM44	TPA	17 Mar 2025

2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certification is traceable to the International System of Unit.


Remark : TPA : Technology Promotion Association (Thailand - Japan)

Result of Calibration :- (*) Without Adjustment

Function of UUC* : Temperature Source

Fresh air setting : Not Available

Environment during calibration		
	Beginning	Finished
Temp. (°C)	24	25
REL.Humid. (%)	50	52
AC Supply (Volt)	221	220

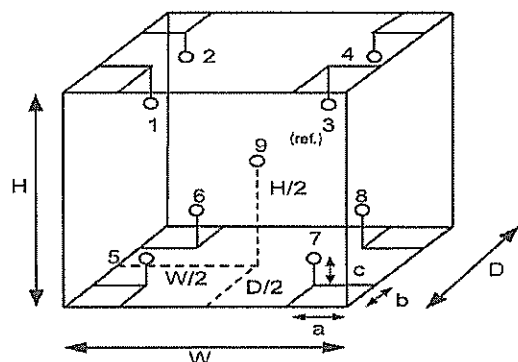

Position :	Ref. Std. ID No.:
1	19RTD-2/1
2	19RTD-2/2
3	19RTD-2/3
4	19RTD-2/4
5	19RTD-2/5
6	24-19RTD-2/6
7	19RTD-2/7
8	19RTD-2/8
9 (ref.)	19RTD-2/9

Probe Installation Details :

a = 10 cm
 b = 10 cm
 c = 10 cm

Dimension of Chamber :

D = 0.48 m
 W = 0.50 m
 H = 1.1 m
 Capacity = 0.26 m³



Equipment : BOD Incubator
Condition As-Received : Used Item
Reference : 2404-0113OC-11
Result of Calibration :- (*) Without Adjustment
Function of UUC* : Temperature Source
Fresh air setting : Not Available

Cert. No.: 24TM702

Page : 3 of 3

Calibration Point (°C)	UUC* Setting (°C)	UUC* Reading (°C)	Temperature stability (± °C)	Temperature uniformity (°C)	Overall Variation (°C)	Coverage Factor <i>k</i>
20.0	20.0	20.0	0.30	0.27	0.77	2

Calibration Point (°C)	Measured Temperature (°C)									Uncertainty (± °C)
	Position									
	1	2	3	4	5	6	7	8	9 (ref.)	
20.0	20.232	20.184	20.129	20.214	20.126	20.102	19.987	20.053	20.128	0.49

Average* : The average of 30 values in each position.

Temperature stability : One-half of the greatest maximum difference of measured temperature at any one sensor.

Temperature uniformity : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.

Overall Variation : The Difference of the maximum and minimum measured temperatures throughout observation.

UUC* : Unit Under Calibration

Note : The reported uncertainty of measurement was included stability and excluded uniformity .

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k* , providing a level of confidence of approximately 95 %.

-o0o-




TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL.0-2717-3000-29 FAX.0-2719-9484



Cert.No.: 24CHO222

Page.: 1 of 3

Certificate of Calibration

Equipment :	Spectrophotometer
Manufacturer :	Labtech
Model :	Blue Star A
Serial No. :	1606UV1507
ID No. :	Ins-LAB-004
Condition As-Received:	Used Item
Received Date :	09 April 2024
Calibration Date :	09 April 2024
Reference :	2404-0113OC-2
Submitted by :	Thai Environmental Technic Limited 1/6 Soi Ramkhamhaeng 145, Khwaeng/Khet Saphan Sung, Bangkok 10240
Calibration Place :	Laboratory (Thai Environment Technic Limited)
Ambient Temperature :	(29.2 - 31.4) °C (On-Site)
Relative Humidity :	(45.2 - 40.3) % (On-Site)
Calibration Procedure :	In - house method : CP-OCH4 based on ASTM E 275-01
Calibrated by :	Saithip Meangmai
Approved by :	 Approved Signatory
() Unnopphol Harachai	
(✓) Ponpan Paipim	
() Saithip Meangmai	
Issue Date :	17 April 2024

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.



Cert. No. : 24CHO222

Page : 2 of 3

Condition of calibration result

1. Reference Standard Material :

<u>Material</u>	<u>Serial No.</u>	<u>Certificate No.</u>	<u>Due date</u>
1. Absorbance Standard set	42527	116226	08 Nov 2025
2. Wavelength Standard set	29829	114509	11 Sep 2025
3. Wavelength Standard set	29829	114510	11 Sep 2025
4. Stray Light Standard set	14004	108964	01 Feb 2025

2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certificate is traceable to the International System of Unit maintained through :

- Starna Scientific Ltd.

4. Spectral BandWidth : 2 nm

Scan Speed : Slow

Calibration Results : without adjustment

Wavelength Accuracy

Certified Values of Reference Material (nm)	UUC Reading (nm)	Uncertainty of Measurement (± nm)	Coverage Factor <i>k</i>
361.00	360.6	0.16	2.00
472.47	471.6	0.16	2.00
536.66	536.2	0.16	2.00
748.48	748.4	0.16	2.00
879.27	879.0	0.16	2.00



Cert. No. : 24CHO222

Page : 3 of 3

Calibration Results : without adjustment

Photometric Accuracy

Wavelength (nm)	Certified Values of Reference Material (Abs)	UUC Reading (Abs)	Uncertainty of Measurement (\pm Abs)	Coverage Factor <i>k</i>
420.0	Zero	0.0002	0.0028	2.00
	0.5739	0.5722	0.0028	2.00
	0.7085	0.7074	0.0030	2.00
	1.0169	1.0146	0.0028	2.00
546.1	Zero	-0.0001	0.0028	2.00
	0.5214	0.5211	0.0028	2.00
	0.6935	0.6926	0.0030	2.00
	0.9978	0.9960	0.0028	2.00
635.0	Zero	0.0000	0.0028	2.00
	0.5626	0.5623	0.0028	2.00
	0.7577	0.7570	0.0030	2.00
	1.0946	1.0927	0.0028	2.00

Stray Light

* Straylight at 260.49 nm \pm 0.11 nm	Reading at 260.49 nm \pm 0.11 nm
Abs	2.2284
%T	0.57

Remark

- Each individual filter is measured against the empty filter holder (blank) used to zero the spectrophotometer
- Cut-off wavelength of stray light reference material (Potassium Iodide) at Wavelength
- Result = Pass, If Absorbance > 2.00 Abs and Transmission < 1.0 %T at Wavelength
- * : Not NSC-ONSC Accredited

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.



A Tresscal company



ID LINE : IEC17025

METROLOGY SYSTEM (THAILAND) CO.,LTD.



Certificate of Calibration

Certificate Number : SPR25040073-1

Page : 1 of 3

Customer : Thai Environmental Technic Limited.

1/6 Soi Ramkhamhaeng 145, Khwaeng Saphan Sung, Khet Saphan
Sung, Bangkok 10240, Thailand.

Equipment Name : Sound Level Meter

Manufacturer : ACO

Model : 6236

Serial Number : 222038

ID. Number : No.70

Environmental Conditions

Ambient Temperature : $23^{\circ}\text{C} \pm 3^{\circ}\text{C}$

Received Date : 04 Apr 2025

Relative Humidity : $50\% \pm 15\%$

Calibration Date : 08 Apr 2025

Location of Calibration : In-Lab

Recommend Due Date : 08 Apr 2026

Calibration Procedure : SP-CPE-04-01

Date of Issue : 09 Apr 2025

Method of Calibration

This certifies that the above instrument was calibrated in compliance with the calibration system requirement of ISO/IEC 17025:2017 in accordance with reference procedure. Standards used to perform this calibration are certified by to NIST or equivalent, National metrology institute, Natural physical constants, consensus standards. The result reported herein apply only to the calibration of the item described above as received. Our decision rule is to contact the customer if the item pass and fail calibration when the results include the uncertainties and the customer must determine if the results meets their needs.

The calibration certificate shall not be reproduced except in full, without written approval of SP Metrology System (Thailand).

Calibrated by : Mr.Nanthawat Wanasit

Approved by :

Calibration Officer

(Ms.Bussakorn Chaikaew)

Authorized Signatory



Calibration Report

Certificate Number : SPR25040073-1

Page : 2 of 3

Reference Standards

Equipment Name	Model	Serial No.	Certificate No.	Due. Date
Sound Level Calibrator	ST-120	211203773	EEL.BP.22/0268	20 Feb 2026

Traceability

This certification is traceable to the International System of Unit maintained at :
TISTR - Thailand Institute of Scientific and Technological Research



Result of Calibration

Certificate Number : SPR25040073-1

Page : 3 of 3

Range : 94 to 114 dB

Function : @1kHz

Select A

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.0	94.0	0.0	0.0	0.15
114	114.3	114.3	0.3	0.3	0.15

Select C

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.0	94.0	0.0	0.0	0.15
114	114.2	114.2	0.2	0.2	0.15

Select Z

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.0	94.0	0.0	0.0	0.15
114	114.2	114.2	0.2	0.2	0.15

Note :

The result of calibration was found accurate as show on date and place of calibration only.
This Certificate is not certified for any commercial transaction.

Measurement Uncertainty

The reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor $k = 2.00$, providing a level of confidence approximately 95%.

- End of Certificate -

Personal Pump Calibration Report

Equipment Type : Personal Pump/Parameter **Barometric pressure (mmHg)** : 758 mmHg

Equipment Range : 0.02-7.00 V/min Temperature (23 ± 3) °C : 25 °C

Calibration Range : 0.02-7.00 U/min Relative Humidity (50±15%) : 55%

Calibration Type : Drycal

Calibration S/N : 4491

[illegible]

Calibration Date 19 / 02 / 68

Calibration By Mesdiana

Remark : Uncertainty Type A = σ = SD

\sqrt{n}
 : SD = Standard deviation
 : \bar{X} = Mean

Personal Pump Calibration Report

Equipment Type : Personal Pump/Parameter *Barometric pressure (mmHg)* : 758 mmHg

Equipment Range : 0.1-7.0 l/min *Temperature (23 ± 3) °C* : 25 °C

Calibration Range : 0.1-4.0 l/min *Relative Humidity (50±15%)* : 55%

Calibration Type : Drycal

Calibration S/N : 4491

Item	Personal	Flow rate	ครั้งที่ 1	ครั้งที่ 2	ครั้งที่ 3	Average	Uncertainty
	S/N	(l/min)					
1.	20151003044	0.20	0.1991	0.1973	0.1975	0.1973	±0.0010
2.	20151003009	0.20	0.1978	0.1979	0.1979	0.1979	±0.0001

Calibration Date 19 / 02 / 68

Calibration By ก้องเกียรติ

Remark : Uncertainty Type A = σ = $\frac{SD}{\sqrt{n}}$

: SD = Standard deviation
: \bar{X} = Mean

Personal Pump Calibration Report

Equipment Type : Personal Pump/Parameter *Barometric pressure (mmHg)* : 758 mmHg

Equipment Range : 0.02-7.00 l/min *Temperature (23 ± 3) °C* : 25 °C

Calibration Range : 0.02-4.00 l/min *Relative Humidity (50±15%)* : 55%

Calibration Type : Drycal

Calibration S/N : 4491

Item	Personal	Flow rate	ครั้งที่ 1	ครั้งที่ 2	ครั้งที่ 3	Average	Uncertainty
	S/N	(l/min)					
1.	20151003041	0.06	0.0592	0.0594	0.0596	0.0594	±0.0002
2.	20151102080	0.06	0.0596	0.0597	0.0598	0.0597	±0.0001

Calibration Date 19 / 02 / 68

Calibration By กิตติศักดิ์

Remark : Uncertainty Type A = σ = $\frac{SD}{\sqrt{n}}$

: SD = Standard deviation
: \bar{X} = Mean

Personal Pump Calibration Report

Equipment Type : Personal Pump/Parameter *Barometric pressure (mmHg)* : 758 mmHg

Equipment Range : 0.02-7.00 l/min *Temperature (23 ± 3) °C* : 25 °C

Calibration Range : 0.02-4.00 l/min *Relative Humidity (50±15%)* : 55%

Calibration Type : Drycal

Calibration S/N : 4491

Item	Personal	Flow rate	ครั้งที่ 1	ครั้งที่ 2	ครั้งที่ 3	Average	Uncertainty
	S/N	(l/min)					
1.	20151003042	0.06	0.0591	0.0591	0.0592	0.0591	±0.0001
2.	20151003043	0.06	0.0596	0.0597	0.0599	0.0598	±0.0002

Calibration Date 19 / 02 / 68

Calibration By ก้องเกียรติศักดิ์

Remark : Uncertainty Type A = σ = SD

$$\sqrt{n}$$

: SD = Standard deviation

: \bar{X} = Mean

Personal Pump Calibration Report

Equipment Type : Personal Pump/Parameter *Barometric pressure (mmHg)* : 758 mmHg

Equipment Range : 0.1-7.0 l/min *Temperature (23 ± 3) °C* : 25 °C

Calibration Range : 0.1-4.0 l/min *Relative Humidity (50±15%)* : 55%

Calibration Type : Drycal

Calibration S/N : 4491

Item	Personal	Flow rate	ครั้งที่ 1	ครั้งที่ 2	ครั้งที่ 3	Average	Uncertainty
	S/N	(l/min)					
1.	20151002115	0.2	0.1992	0.1992	0.1994	0.1992	±0.0001
2.	20180803005	0.2	0.1994	0.1996	0.1998	0.1996	±0.0002

Calibration Date 31 / 03 / 68

Calibration By เกียรติศักดิ์

Remark : Uncertainty Type A = σ = SD

$$\sqrt{n}$$

: SD = Standard deviation

: \bar{X} = Mean

Personal Pump Calibration Report

Equipment Type : Personal Pump/Parameter *Barometric pressure (mmHg)* : 760 mmHg

Equipment Range : 0.1-7.0 l/min *Temperature (23 ± 3) °C* : 25 °C

Calibration Range : 0.1-4.0 l/min *Relative Humidity (50±15%)* : 55%

Calibration Type : Drycal

Calibration S/N : 4491

Item	Personal	Flow rate	ครั้งที่ 1	ครั้งที่ 2	ครั้งที่ 3	Average	Uncertainty
	S/N	(l/min)					
1.	20180806027	0.2	0.1972	0.1973	0.1974	0.1973	±0.0001
2.	20180806018	0.2	0.1976	0.1977	0.1978	0.1977	±0.0001

Calibration Date 21 / 04 / 68

Calibration By วิวัฒน์ศักดิ์

Remark : Uncertainty Type A = σ = SD

$$\sqrt{n}$$

: SD = Standard deviation

: \bar{X} = Mean

Personal Pump Calibration Report

Equipment Type : Personal Pump/Parameter *Barometric pressure (mmHg)* : 758 mmHg

Equipment Range : 0.1-7.0 V/min Temperature (23 ± 3) °C : 25 °C

Calibration Range : 0.1-4.0 V/min Relative Humidity (50±15%) : 55%

Calibration Type : Drycal

Calibration S/N : 4491

[illegible]

Calibration Date 13 / 05 / 68

Calibration By โกศลศักดิ์

Remark : Uncertainty Type A = σ = SD

\sqrt{n}

: SD = Standard deviation

$$\bar{X} = \text{Mean}$$

Personal Pump Calibration Report

Equipment Type : Personal Pump/Parameter *Barometric pressure (mmHg)* : 760 mmHg

Equipment Range : 0.1-7.0 l/min *Temperature (23 ± 3) °C* : 25 °C

Calibration Range : 0.1-4.0 l/min *Relative Humidity (50±15%)* : 55%

Calibration Type : Drycal

Calibration S/N : 4491

Item	Personal	Flow rate	ครั้งที่ 1	ครั้งที่ 2	ครั้งที่ 3	Average	Uncertainty
	S/N	(l/min)					
1.	20180806018	0.2	0.1975	0.1977	0.1979	0.1977	±0.0001
2.	20180802087	0.2	0.1977	0.1978	0.1979	0.1978	±0.0001

Calibration Date 16 / 05 / 68

Calibration By เลิศศักดิ์

Remark : Uncertainty Type A = $\sigma = \frac{SD}{\sqrt{n}}$

: SD = Standard deviation

: \bar{X} = Mean

Personal Pump Calibration Report

Equipment Type : Personal Pump/Parameter **Barometric pressure (mmHg)** : 758 mmHg

Equipment Range : 0.02-7.00 V/min Temperature (23 ± 3) °C : 25 °C

Calibration Range : 0.02-4.00 V/min Relative Humidity (50±15%) : 55%

Calibration Type : Drycal

Calibration S/N : 4491

[illegible]

Calibration Date 05 / 06 / 68

Calibration By meetha

Remark : Uncertainty Type A = σ = SD

\sqrt{n}

: SD = Standard deviation

$$\bar{X} = \text{Mean}$$

Personal Pump Calibration Report

Equipment Type : Personal Pump/Parameter Barometric pressure (mmHg) : 758 mmHg

Equipment Range : 0.02-7.00 V/min Temperature (23 ± 3) °C : 25 °C

Calibration Range : 0.02-4.00 V/min Relative Humidity (50±15%) : 55%

Calibration Type : Drycal

Calibration S/N : 4491

[illegible]

Calibration Date 05 / 06 / 68

Calibration By Inspector

Remark : Uncertainty Type A = σ = SD

$$\sqrt{12}$$

: SD = Standard deviation

$$\therefore \bar{X} = \text{Mean}$$

Personal Pump Calibration Report

Equipment Type : Personal Pump/Parameter *Barometric pressure (mmHg)* : 758 mmHg

Equipment Range : 0.02-7.00 l/min Temperature (23 ± 3) °C : 25 °C

Calibration Range : 0.02-7.00 V/min Relative Humidity (50±15%) : 55%

Calibration Type : Drycal

Calibration S/N : 4491

[illegible]

Calibration Date 05 / 06 / 68

Calibration By Inspector

Remark : Uncertainty Type A = σ = SD

\sqrt{n}

: SD = Standard deviation

$$\bar{X} = \text{Mean}$$

Personal Pump Calibration Report

Equipment Type : Personal Pump/Parameter *Barometric pressure (mmHg)* : 758 mmHg

Equipment Range : 0.1-7.0 V/min *Temperature (23 ± 3) °C* : 25 °C

Calibration Range : 0.1-4.0 V/min *Relative Humidity (50±15%)* : 55%

Calibration Type : Drycal

Calibration S/N : 4491

Item	Personal	Flow rate	ครั้งที่ 1	ครั้งที่ 2	ครั้งที่ 3	Average	Uncertainty
	S/N	(V/min)					
1.	20180802087	0.20	0.1971	0.1971	0.1972	0.1971	±0.0001
2.	20151002115	0.20	0.1981	0.1983	0.1985	0.1983	±0.0002

Calibration Date 13 / 06 / 68

Calibration By ปณิธิศักดิ์

Remark : Uncertainty Type A = σ = SD

$$\sqrt{n}$$

: SD = Standard deviation

: \bar{X} = Mean