

ภาคผนวก ง

---

เอกสารสอบเทียบเครื่องมือ

## CERTIFICATE OF CALIBRATION

Certificate No.: COF-039-67

Page 1 of 2 Pages

**MEASUREMENT ITEM:** Top Load Office  
**MANUFACTURER:** TSC  
**MODEL/TYPE:** TC-5025A  
**SERIAL NUMBER:** 3383  
**ID NUMBER:** UAE.EFM.161/2561  
**CONDITION AS-RECEIVED:** Used Item  
**CUSTOMER:** United Analyst and Engineering Consultant Co., Ltd.  
81 Soi Udomsak 41, Sukhumvit Road, Bangkok, Phrakhanong,  
Bangkok 10260

**RECEIVED DATE:** 16 Sep 2024  
**MEASUREMENT DATE:** 27 Sep 2024  
**ISSUE DATE:** 27 Sep 2024

### ENVIRONMENTAL CONDITIONS:

Ambient condition in the laboratory are as follow:

Temperature:  $23.0 \pm 3.0$  °C  
Relative Humidity:  $55.0 \pm 15.0$  %RH  
Atmospheric Pressure:  $1020 \pm 10$  hPa

### CALIBRATION CONDITION:

Preconditioning: 24 hours at ambient conditions.  
Measurement Condition: The average values during measurement are  $23.9$  °C and  $49.0$  %RH.

**Calibration procedure:**  
The Office gas flow device was calibrated against Standard Rotary Displacement Meter (Rouss Meter) Model G63/IMC/Wide. The IMC-004 was used as a calibration guideline.

**Traceability:**  
This certificate provides a traceability of the measurement to recognized the national standards and to realization of the international system of units (SI) through the NIMT (National Metrology Institute of Thailand) via Certificate number: IMV0069-23.

**Uncertainty of Measurement:**  
The reported uncertainty of measurement is based on the standard uncertainty multiplied by a coverage factor  $k=2$ , which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty has been determined in accordance with the GUM (Evaluation of measurement data - Guide to the expression of uncertainty in measurement).

NOTE: The certificate is valid only to the item calibrated on date and place of calibration.

### TABULATION OF RESULTS:

The table on next page give the measured values.

Calibrated by:

☐ Mr. Satevit Thachad  
37 Makkasajorn Lertnongthol



Approved sign:

Calibration Department Manager

THIS CERTIFICATE REPORT MAY NOT BE REPRODUCED EXCEPT IN FULL UNLESS PERMISSION FOR REPRODUCTION IN WRITING FROM THE LABORATORY

เอกสารไม่ควบคุม  
B 0250406



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)  
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES  
5344 PATTANAKARN ROAD SOI 18, SUANLIANG, SUANLIANG, BANGKOK 10250  
TEL: 6-2715-3066-24 FAX: 6-2719-9484

## Certificate of Calibration

Certificate No.: 25P112  
Page: 1 of 2

**Equipment:** U-Tube Manometer

**Manufacturer:** Dwyer

**Model:** 121-36-WIM

**Serial No.:** -

**ID No.:** UAE.EFM.161/2561

**Condition As-Received:** Used Item

**Received Date:** 10 February 2025

**Calibration Date:** 19 February 2025

**Reference:** 2502-0083WSC

**Ambient Temperature:**  $(23 \pm 2)$  °C

**Relative Humidity:**  $(50 \pm 15)$  %

**Atmospheric Pressure:** 1012 mbar

**Submitted by:** United Analyst and Engineering Consultant Co., Ltd.

81 Soi Udomsak 41, Sukhumvit Road, Bangkok,  
Phrakhanong, Bangkok 10260

**Procedure used:** The calibration was conducted by direct comparison method against Pressure Measuring Instruments Standard according to In-house calibration procedure CP-P04, using "DKD-R 6-1; Calibration of Pressure Gauges, Edition 03/2014" as a guidelines.

### Condition of this result of calibration

1. Reference standards instruments:

Instrument	Model	Serial No.	Certificate No.	Due Date
1) Pressure Calibrator	PC106P	1189	MP-0113-24	10 Jul 2025

2. This result of calibration was made on requested at the point specified by customer.

3. Scale and conversion factor is 1 kPa = 4.0146293 inH<sub>2</sub>O

4. This instrument was used clean air as pressure media.

5. This instrument was installed in vertical orientation and center of connector was used as the reference level.

6. The certificate is valid only to the item calibrated on date and place of calibration.

7. This Certification is traceable to the International System of Unit maintained at:-

-National Institute of Metrology Thailand (NIMT)

Calibrated by: Nopparat Phongam

Issue Date: 21 February 2025

Approved Signatory: Attapol P.

☐ Phalinee Prabsalpa

☐ Sura Suwanasri

☒ Attapol Panurach

เอกสารไม่ควบคุม  
B 0250406

Continuation of Certificate of Calibration Number COF-039-67

Page 2 of 2 Pages

### MEASUREMENT RESULTS:

The Office gas flow device was calibrated by direct comparison method with the Standard Rotary Displacement Meter (Rouss Meter). The humid air used as a medium in the system. The standard conditions are 25°C (298.15 K) and 760 mmHg for standard temperature and standard pressure respectively.

Table 1: The results of Q standard calibration data

Plate	Flow rate m <sup>3</sup> /min	Pressure (Pa) mmHg	Temperature (T <sub>a</sub> ) °C	Temperature (T <sub>m</sub> ) °C	Ap_meter mmHg	Ap_Offset inH <sub>2</sub> O	Y	Standard Flow [Q <sub>s</sub> ] m <sup>3</sup> /min
1	0.703	758.133	22.92	22.49	56.556	1.738	1.319	0.674
2	1.000	758.205	23.70	22.81	83.034	1.473	1.865	0.922
3	1.121	758.264	23.64	22.69	83.633	1.582	2.037	1.064
4	1.167	758.274	23.64	22.65	81.359	1.197	2.382	1.123
5	1.409	758.325	24.00	23.14	80.402	7.654	7.768	1.318

Slope (m): 2.85377

Intercept (b): -0.03807

Correlation coefficient (r): 0.99985

Uncertainty (k=2): 0.015 m<sup>3</sup>/min

Table 2: The results of Q actual calibration data

Plate	Flow rate m <sup>3</sup> /min	Pressure (Pa) mmHg	Temperature (T <sub>a</sub> ) °C	Temperature (T <sub>m</sub> ) °C	Ap_meter mmHg	Ap_Offset inH <sub>2</sub> O	Y	Standard Flow [Q <sub>s</sub> ] m <sup>3</sup> /min
1	0.703	758.133	22.92	22.49	56.556	1.738	0.825	0.673
2	1.000	758.205	23.70	22.81	83.034	1.473	1.166	0.920
3	1.121	758.264	23.64	22.69	83.633	1.582	1.348	1.061
4	1.167	758.274	23.64	22.65	81.359	1.197	1.426	1.123
5	1.409	758.325	24.00	23.14	80.402	7.654	1.732	1.317

Slope (m): 1.26763

Intercept (b): -0.01756

Correlation coefficient (r): 0.99985

Uncertainty (k=2): 0.015 m<sup>3</sup>/min

\*\*\*End of Certificate of Calibration\*\*\*



เอกสารไม่ควบคุม



Cert.No.: 25P112  
Page: 2 of 2

Result of calibration:- Without adjustment

Function:- Pressure Measurement

Increasing Pressure

Range: 0 inH<sub>2</sub>O to 36 inH<sub>2</sub>O

Scale Interval: 0.1 inH<sub>2</sub>O (The Fifth Estimate)

Applied Pressure (inH <sub>2</sub> O)	UUC Indication		ΔP (inH <sub>2</sub> O)	Error (inH <sub>2</sub> O)
	High-port side (inH <sub>2</sub> O)	Low-port side (inH <sub>2</sub> O)		
0.00	0.00	0.00	0.00	0.00
2.00	1.00	-0.98	1.98	-0.02
4.00	2.00	-1.96	3.96	-0.02
6.00	3.00	-3.02	6.02	0.02
8.00	4.00	-4.02	8.02	0.02
10.00	5.00	-5.04	10.04	0.04
12.00	6.00	-6.04	12.04	0.04
14.00	7.00	-7.06	14.06	0.06
16.00	8.00	-8.06	16.06	0.06
18.00	9.00	-9.06	18.06	0.06
20.00	10.00	-10.06	20.06	0.06
22.00	11.00	-11.08	22.08	0.08
24.00	12.00	-12.08	24.08	0.08
26.00	13.02	-13.10	26.12	0.12
28.00	14.02	-14.10	28.12	0.12
30.00	15.02	-15.10	30.12	0.12
32.00	16.02	-16.10	32.12	0.12
34.00	17.02	-17.08	34.10	0.10
35.50	17.86	-17.92	35.78	0.28

The uncertainty of measurement was  $\pm 0.11$  inH<sub>2</sub>O

\* UUC = Unit Under Calibration

\* ΔP = High-port side - Low-port side

The reported uncertainty of measurement was based on a standard uncertainty multiplied

by a coverage factor  $k=2$ , providing a level of confidence of approximately 95 %.

~00~

Attapol P.

เอกสารไม่ควบคุม  
B 1037943



## Certificate of Calibration

Certificate No.: 25P1380  
Page: 1 of 2

Equipment: Aneroid Barometer

Manufacturer: Barigo

Model: -

Serial No.: -

ID No.: UAE.ANV.125/2550

Condition As-Received: Used Item

Received Date: 04 April 2025

Calibration Date: 17 April 2025

Reference: 2504-019WWS

Submitted by: United Analyst and Engineering Consultant Co., Ltd.

Ambient Temperature: ( 23 ± 2 ) °C

Relative Humidity: ( 50 ± 15 ) %

Atmospheric Pressure: 1005 mbar

This certificate may not be reproduced other than in full,  
except with the prior written approval of the head of  
Corporate Services 3: Equipment Calibration and Testing Services.

81 Soi Udomsuk 41, Sukhumvit Road, Bangkok,  
Phrakhanong, Bangkok 10260

Procedure used: The calibration was conducted by direct comparison method against Pressure Measuring Instruments  
Standard according to calibration procedure CP-P10, using "DKD-R 6-1 : Calibration of Pressure Gauges" as  
a guidelines.

### Condition of this result of calibration

1.Reference standards instruments:

Instrument	Model	Serial No.	Certificate No.	Due Date
1) Standard Barometer	DP142	1422505046	MP-0133-24	15 May 2025
2.This instrument was installed in vertical orientation and center of the dial was used as the reference level.				
3.This result of calibration was made on requested at the point specified by customer.				
4.This result of calibration instrument was in absolute pressure.				
5.This instrument was used clean air as pressure media.				
6.The certificate is valid only to the item calibrated on date and place of calibration.				
7.This Certification is traceable to the International System of Unit maintained through:-				
-National Institute of Metrology Thailand (NIMT)				

Calibrated by: Kaeripon Sanyichai  
Issue Date: 21 April 2025

Approved Signatory:

[ ] Sura Sawannasri  
[✓] Atapol Panurich

เอกสารไม่ควบคุม



## Certificate of Calibration

Certificate No.: 25H812  
Page: 1 of 2

Equipment: Dial Thermo-Hygrometer

Manufacturer: Barigo

Model: -

Serial No.: -

ID No.: UAE.ANV.132/2550

Condition As-Received: Used Item

Received Date: 04 April 2025

Calibration Date: 10 April 2025  
to 17 April 2025

Reference: 2504-019WWS

Submitted by: United Analyst and Engineering Consultant Co., Ltd.

Ambient Temperature: ( 25 ± 3 ) °C

Relative Humidity: ( 50 ± 20 ) %

This certificate may not be reproduced other than in full,  
except with the prior written approval of the head of  
Corporate Services 3: Equipment Calibration and Testing Services.

81 Soi Udomsuk 41, Sukhumvit Road, Bangkok,  
Phrakhanong, Bangkok 10260

Procedure used: Calibration were conducted using in-house calibration procedure CP-H02 according to comparison  
with standard chilled mirror sensor for humidity measurement function and comparison with standard  
temperature probe for temperature measurement function into humidity / temperature chamber.

### Condition of this result of calibration

1.Reference standards instruments:

Instrument	Model	Serial No.	Certificate No.	Due Date
1) Dew Point Hygrometer	Optidew 401	164756	TH-0005-25	05 Feb 2026
2) Handheld Thermometer With Sensor	1523	5717096	2411241	16 Nov 2025
2.The certificate is valid only to the item calibrated on date and place of calibration.				
3.This Certification is traceable to the International System of Unit maintained through:-				
-National Institute of Metrology (Thailand), NSG-ONSC Accredited No. Calibration 0144				
-Technology Promotion Association (Thailand-Japan), NSG-ONSC Accredited No. Calibration 0008				

Calibrated by: Somchai Dumvor  
Issue Date: 18 April 2025

Approved Signatory:

[ ] Chaitri Waewarajus  
[ ] Pomsitippe Taneyasakul  
[✓] Viporn Tantiyawutti

เอกสารไม่ควบคุม



Cert.No.: 25P1380  
Page: 2 of 2

Result of calibration:- Without adjustment  
Function: Absolute Pressure Measurement

Range: 960 hPa to 1030 hPa  
Scale Interval: 1 hPa ( The Fifth Estimate )

Increasing Pressure

Applied Pressure (hPa)	961.40	971.90	981.62	992.25	1001.35	1009.76	1019.56	1029.44
UUC* Indication (hPa)	960.0	970.0	980.0	990.0	1000.0	1010.0	1020.0	1030.0
Error (hPa)	-1.40	-1.90	-1.62	-2.25	-1.35	0.24	0.44	0.56

Decreasing Pressure

Applied Pressure (hPa)	1029.44	1019.30	1009.48	1000.54	991.38	981.80	971.62	961.62
UUC* Indication (hPa)	1030.0	1020.0	1010.0	1000.0	990.0	980.0	970.0	960.0
Error (hPa)	0.56	0.70	0.52	-0.54	-1.38	-1.80	-1.62	-1.62

The uncertainty of measurement was ± 0.25 hPa

\* UUC = Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied  
by a coverage factor k = 2, providing a level of confidence of approximately 95 %

-000-



Cert. No.: 25H812  
Page: 2 of 2

Result of Calibration:- Without Adjustment  
Function: Humidity Measurement

Reference Temperature (°C)	Standard Humidity (%R.H.)	UUC* Reading (%R.H.)	Correction (%R.H.)	Uncertainty of Measurement (±%R.H.)
25.0	40.1	42	-1.9	1.7
25.0	60.0	60	0.0	1.6
25.0	80.0	78	4.0	1.9

Result of Calibration:- Without Adjustment  
Function: Temperature Measurement

Standard Temperature (°C)	UUC* Reading (°C)	Correction (°C)	Uncertainty of Measurement (±°C)
20.001	21.0	-0.999	0.72
24.987	25.0	-0.013	0.72
30.021	30.0	0.021	0.72
34.964	34.0	0.964	0.72
40.032	39.0	1.032	0.72

UUC\* : Unit Under Calibration

The reported uncertainty of measurement was base on standard uncertainty multiplied  
by coverage factor k = 2.00, providing confidence level approximately 95%.

-000-

เอกสารไม่ควบคุม

เอกสารไม่ควบคุม



# THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804, 0-2399-0469

## Calibration Certificate

Issued by : Calibration & Test Section : Meteorological Instruments Bureau

Date of Issue 18 March, 2025

Certification No. 162/25

Page : 1 of 5

Object : Wind Speed & Wind Direction Data Logger

Manufacturer : SCARLET/TECH

Type : WL-21

Mfg Code : Wireless Receiver 2111DR0041

Wind Sensor 2111DT0041

Customer : United Analyst and Engineering Consultant Co., Ltd.

81 Soi Udomsuk 41, Sukhumvit Road,

Bangchak, Prakanong, Bangkok 10260.

Calibration Condition : Temperature 25.1 °C Barometric Pressure 1011.4 hPa

NATIONAL STANDARD WIND TUNNEL : Vane Angel Bench Stand Model 18112

: Micromanometer Theodor Friedrichs FC014 Serial No. 9310119 : HOOK GAGE NO 1425

N.I.S.T. Test Reference Number 731241460 : Standard Velocity at 20 - 30 m/sec

: Ultrasonic Anemometer Model DA-850-3TV (sensor TR-90AH)

Serial Number 110730029 (sensor 120629586)

JAPAN QUALITY ASSURANCE ORGANIZATION : Standard Velocity at 0 - 20 m/sec

STANDARD THERMOMETER : Theodor Friedrich : Dry No.8390/94 Wet No. 8389/94

: testo, testo 645 Serial No. 02049057 : Thermoschneider No.918802

STANDARD BAROMETER : Digital Barometer Vaisala Type PTB220 No. V1220015

Barometer Vaisala Type PTB330 No. 84320001

Calibrated by

Mr. Watchara

Mechanical Engineer

(Authorized Signature)

for the Chief

Sub-Standard Instrument

เอกสารไม่ควบคุม



# THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804, 0-2399-0469

## The Result of Calibration

Certification No. 162/25

18 March, 2025

Page : 4 of 5

Standard Barometer	Tested Barometer	Correction
Pressure	Pressure	mmHg
756.93	757	-0.07
757.10	757	0.10
757.31	757	0.31
757.72	758	-0.28
757.36	757	0.36
757.81	758	-0.19
758.54	759	-0.46
758.43	758	0.43
754.71	755	-0.29
754.82	756	-0.18
754.88	755	-0.12
755.57	756	-0.43
755.68	756	-0.32
755.99	756	-0.01
757.23	757	0.23
756.06	756	0.06
758.99	757	-0.01
758.09	758	0.09
755.94	756	-0.06
757.19	757	0.19

Average

Mechanical Engineer

Calibration & Test Section  
Meteorological Instruments Bureau

เอกสารไม่ควบคุม



# THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804, 0-2399-0469

## The Result of Calibration

Certification No. 162/25

18 March, 2025

Page : 2 of 5

Standard		HOOK GAGE NO. 1425		TESTED ANEMOMETER	
Ultrasonic Anemometer	Pressure	Vacuum	Velocity	Velocity	Correction
m/sec	inches H2O	mm Hg	ft/min	m/sec	m/sec
1.00	-	-	-	1.0	0.00
3.02	-	-	-	3.0	0.02
5.00	-	-	-	5.0	0.00
7.04	-	-	-	7.0	0.04
9.02	-	-	-	8.9	0.12
11.02	-	-	-	11.0	0.02
13.01	-	-	-	12.9	0.11
15.01	-	-	-	15.0	0.01
17.02	-	-	-	17.0	0.02
20.02	-	-	-	20.0	0.02

Vane Angel Bench Stand Model 18112

Young Meteorological Instruments

WIND DIRECTION	TESTED WIND DIRECTION
0	0
90	90
180	180
270	270

Calibrated by

Mechanical Engineer

Calibration & Test Section  
Meteorological Instruments Bureau

เอกสารไม่ควบคุม



# THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804, 0-2399-0469

## The Result of Calibration

Certification No. 162/25

18 March, 2025

Page : 3 of 5

Standard Barometer	Tested Barometer	Correction
Pressure	Pressure	mbar
1009.16	1010	-0.84
1009.39	1009	0.39
1009.66	1009	0.66
1010.21	1010	0.21
1009.73	1010	-0.27
1010.33	1010	0.33
1011.31	1011	0.31
1011.16	1011	0.16
1006.20	1006	0.20
1006.34	1006	0.34
1006.43	1006	0.43
1007.35	1007	0.35
1007.49	1007	0.49
1007.91	1008	-0.09
1009.56	1009	0.56
1008.00	1008	0.00
1009.24	1009	0.24
1010.71	1011	-0.29
1007.84	1008	-0.16
1009.51	1009	0.51

Average

Calibrated by

Mechanical Engineer

Calibration & Test Section  
Meteorological Instruments Bureau

เอกสารไม่ควบคุม



# THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804,0-2399-0469

## The Result of Calibration

Certification No. 162/25

18 March, 2025

Page : 5 of 5

Standard Temp. °C	Temperature Sensor Reading	
	Reading °C	Correction °C
45.3	45	0.3
39.4	39	0.4
15.4	15	0.4

Calibration



Mechanical Engineer



เอกสารไม่ควบคุม



# THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804,0-2399-0469

## The Result of Calibration

Certification No. 112/25

19 February, 2025

Page : 2 of 5


Standard Ultrasonic Anemometer m/sec	HOOK GAGE NO. 1425			TESTED ANEMOMETER	
	Pressure inches H2O	Vacuum inches H2O	Velocity m/sec	Velocity m/sec	Correction m/sec
1.00	-	-	-	1.0	0.00
3.02	-	-	-	3.0	0.02
5.00	-	-	-	5.0	0.00
7.04	-	-	-	7.0	0.04
9.02	-	-	-	9.0	0.02
11.02	-	-	-	11.0	0.02
13.01	-	-	-	13.0	0.01
15.01	-	-	-	15.0	0.01
17.02	-	-	-	17.0	0.02
20.02	-	-	-	20.0	0.02

Vane Angel Bench Stand Model 18112

Young Meteorological Instruments

WIND DIRECTION	TESTED WIND DIRECTION
0	0
90	90
180	180
270	270

Calibration



Mechanical Engineer



เอกสารไม่ควบคุม



# THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804,0-2399-0469

## Calibration Certificate

Issued by : Calibration & Test Section : Meteorological Instruments Bureau

Date of Issue : 19 February, 2025

Certification No. 112/25

Page : 1 of 5

Object : Wind Speed & Wind Direction Data Logger

Manufacturer : SCARLET/TECH

Type : WL-21

Mfg Code : Wireless Receiver : 2111DR0052

Wind Sensor : 2111DT0052

Customer : United Analyst and Engineering Consultant Co.,Ltd.

81 Soi Udomsuk 41, Sukhumvit Road,

Bangchak, Prakanong, Bangkok 10260.

Calibration Condition : Temperature : 25.1 °C : Barometric Pressure : 1012.3 hPa

NATIONAL STANDARD WIND TUNNEL : Wind Aft Plotting Board

: Micromanometer : Theodor Friedrich FC014 Serial No. 9310119 : HOOK GAGE NO 1425

N.I.S.T. Test Reference Number : 731/241469 : Standard Velocity at 20 - 30 m/sec

: Ultrasonic Anemometer : Model DA-650-3TV (sensor TR-90AH)

Serial Number 110730029 (sensor 120629586)

JAPAN QUALITY ASSURANCE ORGANIZATION : Standard Velocity at 0 - 20 m/sec

STANDARD THERMOMETER : Theodor Friedrich : Dry No.8390/94 Wet No. 8389/94

: Testo, testo 545 Serial No. 02048057 : Thermoschneider No.918802

STANDARD BAROMETER : Digital Barometer Vaisala Type PTB220 No. V1220015

: Digital Barometer Vaisala Type PTB220 No. V1220015



Mechanical Engineer

(Authorised Signatory)

for the Chief

Sub-Standard Instrument

เอกสารไม่ควบคุม



# THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804,0-2399-0469

## The Result of Calibration

Certification No. 112/25


19 February, 2025

Page : 3 of 5

Standard Barometer	Tested Barometer	Correction
Pressure	Pressure	mbar
1012.05	1012	0.05
1011.25	1011	0.25
1012.92	1013	-0.08
1010.09	1010	0.09
1008.87	1009	-0.13
1010.43	1011	-0.57
1011.39	1011	0.39
1011.05	1011	0.05
1010.72	1011	-0.28
1010.30	1010	0.30
1009.81	1010	-0.19
1008.93	1009	-0.07
1009.35	1009	0.35
1009.89	1010	-0.11
1010.57	1010	0.57
1011.41	1011	0.41
1012.31	1012	0.31
1009.75	1010	-0.25
1010.67	1011	-0.33
1011.01	1011	0.01

Average : 0.04

Calibration



Mechanical Engineer



เอกสารไม่ควบคุม



# THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804,0-2399-0469

## The Result of Calibration

Certification No. 112/25

19 February, 2025

Page : 4 of 5

Standard Barometer	Tested Barometer	Correction
Pressure	Pressure	mmHg
759.10	759	0.10
758.50	758	0.50
759.75	760	-0.25
757.63	758	-0.37
756.71	757	-0.29
757.88	758	-0.12
758.60	758	0.00
758.35	758	0.35
758.10	758	0.10
757.79	758	-0.21
757.42	757	0.42
756.76	757	-0.24
757.07	757	0.07
757.48	757	0.48
757.99	758	-0.01
758.62	759	-0.38
759.29	759	0.29
757.37	757	0.37
758.06	758	0.06
758.32	758	0.32

Average

0.08

Calibration & Test Section

Meteorological Instruments Bureau

Mechanical Engineer

เอกสารไม่ควบคุม



# THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804,0-2399-0469

## Calibration Certificate

Issued by : Calibration & Test Section : Meteorological Instruments Bureau

Date of Issue : 19 February, 2025

Certification No. 108/25

Page : 1 of 5

Object : Wind Speed & Wind Direction Data Logger

Manufacturer : SCARLET/TECH

Type : WL-21

Mfg Code : Wireless Receiver 2111DR0058

Wind Sensor 2111DT0058

Customer : United Analyst and Engineering Consultant Co.,Ltd.

81 Soi Udomsuk 41, Sukhumvit Road,

Bangchak, Prakanong, Bangkok 10260.

Calibration Condition : Temperature 25.1 °C Barometric Pressure 1012.0 hPa

NATIONAL STANDARD WIND TUNNEL : Wind Aloft Plotting Board

: Micromanometer Theodor Friedrich FC014 Serial No. 9310119 : HOOK GAGE NO 1425

N.I.S.T. Test Reference Number 731/241460 : Standard Velocity at 20 - 30 m/sec

: Ultrasonic Anemometer Model DA-650-3TV (sensor TR-90AH)

Serial Number 110730029 (sensor 120629586)

JAPAN QUALITY ASSURANCE ORGANIZATION : Standard Velocity at 0 - 20 m/sec

STANDARD THERMOMETER : Theodor Friedrich : Dry No.8390/94 Wet No.8389/94

: testo Testo 645 Serial No. 02648057 : Thermoschneider No.918802

STANDARD BAROMETER : Digital Barometer Vaisala Type PTB200 No. V1220015

: Digital Barometer Vaisala Type PTB330 No. K4320001

(Authorised Signatory)

for the Chief

Sub-Standard Instrument

Mechanical Engineer

เอกสารไม่ควบคุม



# THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804,0-2399-0469

## The Result of Calibration

Certification No. 112/25

19 February, 2025

Page : 5 of 5

Standard	Temperature Sensor Reading	
	Reading	Correction
Temp.	°C	°C
45.5	46	-0.5
30.4	30	0.4
15.6	15	0.6

Mechanical Engineer

Calibration & Test Section

Meteorological Instruments Bureau

เอกสารไม่ควบคุม



# THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804,0-2399-0469

## The Result of Calibration

Certification No. 108/25

19 February, 2025

Page : 2 of 5

Standard	HOOK GAGE NO. 1425			TESTED ANEMOMETER	
	Pressure	Vacuum	Velocity	Velocity	Correction
Ultrasonic Anemometer	m/sec	inches H2O	inches H2O	m/sec	m/sec
1.00	-	-	-	1.0	0.00
3.02	-	-	-	3.0	0.02
5.00	-	-	-	5.0	0.00
7.04	-	-	-	7.0	0.04
9.02	-	-	-	9.0	0.02
11.02	-	-	-	11.0	0.02
13.01	-	-	-	12.9	0.11
15.01	-	-	-	15.0	0.01
17.02	-	-	-	17.0	0.02
20.02	-	-	-	20.0	0.02

Vane Angel Bench Stand Model 18112

Young Meteorological Instruments

WIND DIRECTION	TESTED WIND DIRECTION
0	0
90	90
180	180
270	

Cal

Mechanical Engineer

Calibration & Test Section

Meteorological Instruments Bureau

เอกสารไม่ควบคุม



# THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804, 0-2399-0469

## The Result of Calibration

Certification No. 108/25

Page : 3 of 5

19 February, 2025

Standard Barometer	Tested Barometer	Correction
Pressure	Pressure	mbar
1012.05	1012	0.05
1011.25	1011	0.25
1012.92	1013	-0.08
1010.09	1010	0.09
1008.87	1009	-0.13
1010.43	1010	0.43
1011.39	1011	0.39
1011.05	1011	0.05
1010.72	1011	-0.28
1010.30	1010	0.30
1009.81	1010	-0.19
1008.90	1009	-0.07
1009.35	1009	0.35
1009.89	1010	-0.11
1010.57	1011	-0.43
1011.41	1012	-0.59
1012.31	1012	0.31
1009.75	1010	-0.25
1010.67	1011	-0.33
1011.01	1011	0.01

Average

Cal

Mechanical Engineer

Calibration & Test Section  
Meteorological Instruments Bureau

เอกสารไม่ควบคุม



# THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804, 0-2399-0469

## The Result of Calibration

Certification No. 108/25

Page : 5 of 5

19 February, 2025

Standard Temp. °C	Temperature Sensor Reading	
	Reading °C	Correction °C
45.5	45	0.5
30.4	30	0.4
15.6	15	-0.4

C

Mechanical Engineer

Calibration & Test Section  
Meteorological Instruments Bureau

เอกสารไม่ควบคุม



# THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804, 0-2399-0469

## The Result of Calibration

Certification No. 108/25

Page : 4 of 5

19 February, 2025

Standard Barometer	Tested Barometer	Correction
Pressure	Pressure	mmHg
759.10	759	0.10
758.50	759	-0.50
759.75	760	-0.25
757.63	758	-0.37
756.71	757	-0.29
757.88	758	-0.12
756.60	759	-0.40
758.35	758	0.35
758.10	758	0.10
757.79	758	-0.21
757.42	757	0.42
756.76	757	-0.24
757.07	757	0.07
757.48	758	-0.52
757.99	758	-0.01
758.62	758	0.62
759.29	759	0.29
757.37	757	0.37
758.06	758	0.06
758.32	758	0.32

Average

Mechanical Engineer

Calibration & Test Section  
Meteorological Instruments Bureau

เอกสารไม่ควบคุม



# THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804, 0-2399-0469

## Calibration Certificate

Issued by : Calibration & Test Section : Meteorological Instruments Bureau

Date of Issue : 3 January, 2025

Certification No. 001/25

Page : 1 of 5

Object : Wind Speed & Wind Direction Data Logger

Manufacturer : SCARLET/TECH

Type : WL-21

Mfg Code : Wireless Receiver 2111DR0072

Wind Sensor 2111DR0072

Customer : United Analyst and Engineering Consultant Co., Ltd.

81 Soi Udomsuk 41, Sukhumvit Road,

Bangchak, Prakanong, Bangkok 10260.

Calibration Condition : Temperature 25.1 °C Barometric Pressure 1012.1 hPa

NATIONAL STANDARD WIND TUNNEL : Wind Axi Plotting Board

: Micromanometer Theodor Friedrichs FC014 Serial No. 9310119 : HOOK GAGE NO 1425

N.I.S.T. Test Reference Number 731/241460

: Standard Velocity at 20 : 30 m/sec

: Ultrasonic Anemometer Model DA-650-3TV (sensor TR-90AH)

Serial Number 110730029 (sensor 120629686)

JAPAN QUALITY ASSURANCE ORGANIZATION : Standard Velocity at 0 - 20 m/sec

STANDARD THERMOMETER : Theodor Friedrichs : Dry No. 8390/94 Wet No. 8389/94

: testo 545 Serial No. 02949057 : Thermoschneider No. 918602

STANDARD BAROMETER : Digital Barometer Vaisala Type PTB220 No. V1220015

ometer Vaisala Type PTB300 No. V14320001

Mechanical Engineer

(Authorized Signatory)

for the Chief

Sub-Standard Instrument

เอกสารไม่ควบคุม



# THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804, 0-2399-0469

## The Result of Calibration

Certification No. 001/25

3 January, 2025

Page : 2 of 5

Standard	HOOK GAGE NO. 1425			TESTED ANEMOMETER	
	Pressure	Vacuum	Velocity	Velocity	Correction
Ultrasonic Anemometer	inches H <sub>2</sub> O	inches H <sub>2</sub> O	m/sec	m/sec	m/sec
1.00	-	-	-	1.0	0.00
3.02	-	-	-	3.0	0.02
5.00	-	-	-	5.0	0.00
7.04	-	-	-	7.0	0.04
9.02	-	-	-	9.0	0.02
11.02	-	-	-	11.0	0.02
13.01	-	-	-	13.0	0.01
15.01	-	-	-	15.0	0.01
17.02	-	-	-	17.1	-0.08
20.02	-	-	-	20.1	-0.08

Vane Angel Bench Stand Model 18112	
Young Meteorological Instruments	
WIND DIRECTION	TESTED WIND DIRECTION
0	0
90	90
180	180
270	

Calibration & Test Section  
Meteorological Instruments Bureau

Mechanical Engineer

เอกสารไม่ควบคุม



# THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804, 0-2399-0469

## The Result of Calibration

Certification No. 001/25

3 January, 2025

Page : 4 of 5

Standard Barometer	Tested Barometer	Correction
Pressure	Pressure	mmHg
759.10	759	0.10
758.50	759	-0.50
759.75	760	-0.25
757.83	758	-0.37
756.71	757	-0.29
757.88	758	-0.12
756.80	759	-0.40
758.35	758	0.35
758.10	758	0.10
757.79	758	-0.21
757.42	757	0.42
756.76	757	-0.24
757.07	757	0.07
757.46	757	0.48
757.99	758	-0.01
758.62	759	-0.38
759.29	759	0.29
757.37	757	0.37
758.06	758	0.06
758.32	758	0.32

Average

Mechanical Engineer

Calibration & Test Section  
Meteorological Instruments Bureau

เอกสารไม่ควบคุม



# THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804, 0-2399-0469

## The Result of Calibration

Certification No. 001/25

3 January, 2025

Page : 3 of 5

Standard Barometer	Tested Barometer	Correction
Pressure	Pressure	mbar
1012.05	1012	0.05
1011.25	1011	0.25
1012.92	1013	-0.08
1010.09	1010	0.09
1008.87	1009	-0.13
1010.43	1010	0.43
1011.39	1011	0.39
1011.05	1011	0.05
1010.72	1011	-0.28
1010.30	1010	0.30
1009.81	1010	-0.19
1008.93	1009	-0.07
1009.35	1009	0.35
1009.89	1010	-0.11
1010.57	1011	-0.43
1011.41	1011	0.41
1012.31	1012	0.31
1009.75	1010	-0.25
1010.67	1011	-0.33
1011.01	1011	0.01

Average

Calibration & Test Section  
Meteorological Instruments Bureau

Mechanical Engineer

เอกสารไม่ควบคุม



# THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804, 0-2399-0469

## The Result of Calibration

Certification No. 001/25

3 January, 2025

Page : 5 of 5

Standard	Temperature Sensor Reading	
	Reading	Correction
Temp. °C	°C	°C
45.5	45	0.5
30.4	30	0.4
15.6	15	-0.4

Mechanical Engineer

Calibration & Test Section  
Meteorological Instruments Bureau

เอกสารไม่ควบคุม

**MULTI-POINT GAS TEST REPORT**


Test Date : Oct 4, 2024

Equipment : Gas Analyzer (NO<sub>2</sub>) Model : 42C  
Manufacturer : Thermo Electron Corporation Serial Number : 42C-0508011076

Standard Gas Concentration			Dilutor Detail	
Sulphur Dioxide (SO <sub>2</sub> )	42.89	PPM	Manufacturer :	Thermo Scientific
Nitric Oxide (NO)	46.77	PPM	Model :	146i
Methane (CH <sub>4</sub> )	-	PPM	Serial Number :	1180540071
Carbon Monoxide (CO)	965.9			
Cylinder No. :	EB0159156			
Expiration Date :	Nov 6, 2026			

**Multi-point gas test data**

Reference Value (ppb)	Analyzer Display (ppb)	Difference Error	Percent Error	[% Error]
Level 1 Zero	0.0	0.00	0.00	0.00
Level 2 20.00%	100.0	100.9	0.90	0.89
Level 3 40.00%	200.0	200.5	0.50	0.25
Level 4 60.00%	300.0	300.8	0.80	0.27
Level 5 80.00%	400.0	400.0	0.00	0.00
Remark : Measuring Range 500.0 ppb		Average Difference (%)		
:Acceptable Limit $\pm$ 5%		0.28		

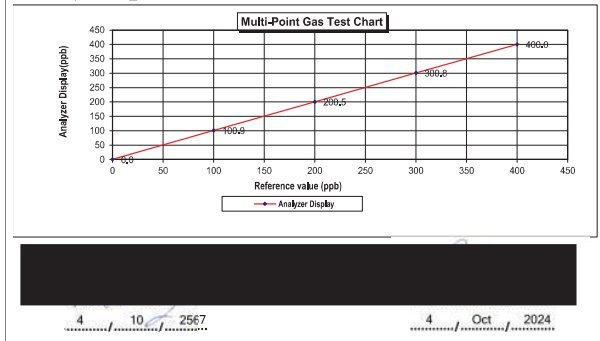

**MULTI-POINT GAS TEST REPORT**


Test Date : Oct 11, 2024

Equipment : Gas Analyzer (NO<sub>2</sub>) Model : 42C  
Manufacturer : Thermo Electron Corporation Serial Number : 0517512001

Standard Gas Concentration			Dilutor Detail	
Sulphur Dioxide (SO <sub>2</sub> )	42.89	PPM	Manufacturer :	Thermo Scientific
Nitric Oxide (NO)	46.77	PPM	Model :	146i
Methane (CH <sub>4</sub> )	-	PPM	Serial Number :	1180540071
Carbon Monoxide (CO)	965.9			
Cylinder No. :	EB0159156			
Expiration Date :	Nov 6, 2026			

**Multi-point gas test data**

Reference Value (ppb)	Analyzer Display (ppb)	Difference Error	Percent Error	[% Error]
Level 1 Zero	0.0	0.00	0.00	0.00
Level 2 20.00%	100.0	101.7	1.70	1.67
Level 3 40.00%	200.0	200.7	0.70	0.35
Level 4 60.00%	300.0	300.8	0.80	0.27
Level 5 80.00%	400.0	400.0	0.00	0.00
Remark : Measuring Range 500.0 ppb		Average Difference (%)		
:Acceptable Limit $\pm$ 5%		0.46		

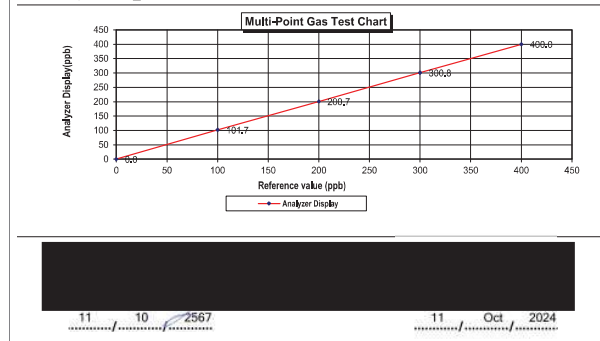

**MULTI-POINT GAS TEST REPORT**


Test Date : Oct 4, 2024

Equipment : Gas Analyzer (NO<sub>2</sub>) Model : 42C  
Manufacturer : Thermo Electron Corporation Serial Number : 0517512000

Standard Gas Concentration			Dilutor Detail	
Sulphur Dioxide (SO <sub>2</sub> )	42.89	PPM	Manufacturer :	Thermo Scientific
Nitric Oxide (NO)	46.77	PPM	Model :	146i
Methane (CH <sub>4</sub> )	-	PPM	Serial Number :	1180540071
Carbon Monoxide (CO)	965.9			
Cylinder No. :	EB0159156			
Expiration Date :	Nov 6, 2026			

**Multi-point gas test data**

Reference Value (ppb)	Analyzer Display (ppb)	Difference Error	Percent Error	[% Error]
Level 1 Zero	0.0	0.00	0.00	0.00
Level 2 20.00%	100.0	100.7	0.70	0.70
Level 3 40.00%	200.0	200.5	0.50	0.25
Level 4 60.00%	300.0	300.9	0.90	0.30
Level 5 80.00%	400.0	400.0	0.00	0.00
Remark : Measuring Range 500.0 ppb		Average Difference (%)		
:Acceptable Limit $\pm$ 5%		0.25		

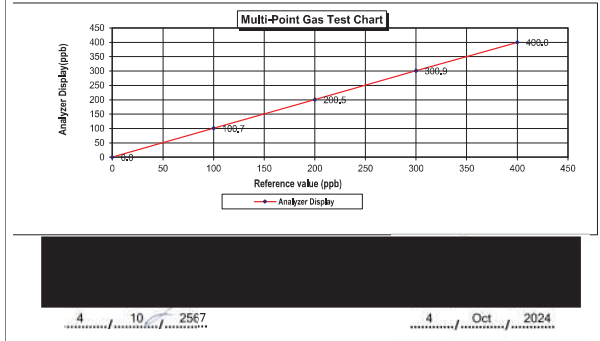

**MULTI-POINT GAS TEST REPORT**


Test Date : Sep 17, 2024

Equipment : Gas Analyzer (NO<sub>2</sub>) Model : 42i  
Manufacturer : Thermo Scientific Serial Number : CM08130002

Standard Gas Concentration			Dilutor Detail	
Sulphur Dioxide (SO <sub>2</sub> )	42.89	PPM	Manufacturer :	Thermo Scientific
Nitric Oxide (NO)	46.77	PPM	Model :	146i
Methane (CH <sub>4</sub> )	-	PPM	Serial Number :	1180540071
Carbon Monoxide (CO)	965.9			
Cylinder No. :	EB0159156			
Expiration Date :	Nov 6, 2026			

**Multi-point gas test data**

Reference Value (ppb)	Analyzer Display (ppb)	Difference Error	Percent Error	[% Error]
Level 1 Zero	0.0	0.50	0.50	0.50
Level 2 20.00%	100.0	101.6	1.60	1.57
Level 3 40.00%	200.0	200.5	0.50	0.25
Level 4 60.00%	300.0	300.8	0.80	0.27
Level 5 80.00%	400.0	400.0	0.00	0.00
Remark : Measuring Range 500.0 ppb		Average Difference (%)		
:Acceptable Limit $\pm$ 5%		0.52		

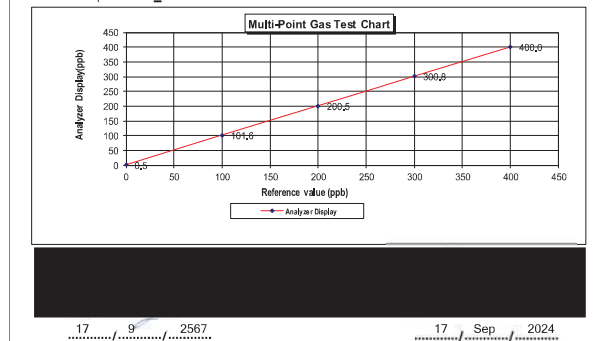

MULTI-POINT GAS TEST REPORT


Test Date : Sep 20, 2024

Equipment : Gas Analyzer (NO<sub>2</sub>) Model : 42i  
Manufacturer : Thermo Scientific Serial Number : CM19050148

Standard Gas Concentration		Dilutor Detail	
Sulphur Dioxide (SO <sub>2</sub> )	42.89 PPM	Manufacturer :	Thermo Scientific
Nitric Oxide (NO)	46.77 PPM	Model :	146i
Methane (CH <sub>4</sub> )	- PPM	Serial Number :	1180540071
Carbon Monoxide (CO)	965.9		
Cylinder No. :	EB0159156		
Expiration Date :	Nov 6, 2026		

Multi-point gas test data

Reference Value (ppb)		Analyzer Display (ppb)	Difference Error	Percent Error	[% Error]
Level 1	Zero	0.0	0.00	0.00	0.00
Level 2	20.00%	100.0	100.7	0.70	0.70
Level 3	40.00%	200.0	200.6	0.30	0.30
Level 4	60.00%	300.0	300.9	0.30	0.30
Level 5	80.00%	400.0	400.0	0.00	0.00
Remark : Measuring Range		500.0 ppb	Average Difference (%)		
			:Acceptable Limit $\pm$ 5%		

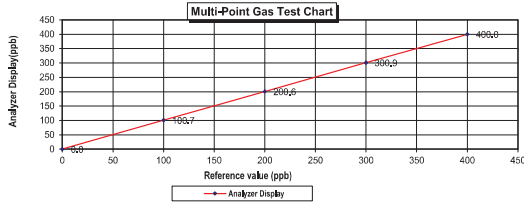

20 9 2567 20 Sep 2024

CERTIFICATE OF ANALYSIS

Grade of Product: EPA PROTOCOL STANDARD

Customer: AIR LIQUIDE (THAILAND) LTD  
Part Number: E04N99E15A01D3  
Cylinder Number: EBO159156  
Laboratory: 124 - Durham (SAP) - NC  
PGVP Number: B22023  
Gas Code: CO,NO,NOX,SO2,BALN  
Reference Number: 122-402880224-1  
Cylinder Volume: 144.0 CF  
Cylinder Pressure: 2015 PSIG  
Valve Outlet: 660  
Certification Date: Nov 06, 2023  
Expiration Date: Nov 06, 2026

Certification performed in accordance with "EPA Traceability Protocol for Assay and Certification of Gaseous Calibration Standards (May 2017)" 4th revised EPC, 600/R-12/01, using the assay procedures listed. Analytical Multi-Point Gas does not require certification for analytical reference. This cylinder has a total analytical uncertainty as stated below with a confidence level of 95%. There are no significant impurities which affect the use of this calibration mixture. All concentrations are on a mole/mole basis unless otherwise noted. The results relate only to the items tested. The report shall not be reproduced except in full without approval of the laboratory. Do Not Use This Cylinder below 100 ppb. i.e. 0.7 megapascals.

Component	Requested Concentration	Actual Concentration	Protocol Method	Total Relative Uncertainty	Assay Dates
NOX	45.00 PPM	46.78 PPM	G1	$\pm$ 1.3% NIST Traceable	10/30/2023, 11/06/2023
NITRIC OXIDE	45.00 PPM	46.77 PPM	G1	$\pm$ 1.3% NIST Traceable	10/30/2023, 11/06/2023
SULFUR DIOXIDE	45.00 PPM	42.89 PPM	G1	$\pm$ 1.0% NIST Traceable	10/30/2023, 11/06/2023
CARBON MONOXIDE	1000 PPM	965.9 PPM	G1	$\pm$ 0.7% NIST Traceable	10/30/2023, 11/06/2023
NITROGEN	Balance				

Type	Lot ID	Cylinder No	Concentration	Uncertainty	Expiration Date
NTRM	21060703	CC707954	48.41 PPM NITRIC OXIDE/NITROGEN	$\pm$ 1.2%	Sep 21, 2025
PRM	PRM	D913660	15.01 PPM NITROGEN DIOXIDE/AIR	$\pm$ 1.5%	Feb 18, 2023
QMS	124266889	CC322689	4.873 PPM NITROGEN DIOXIDE/NITROGEN	$\pm$ 1.8%	Feb 17, 2026
NTRM	18061005	CC473180	48.02 PPM SULFUR DIOXIDE/NITROGEN	$\pm$ 0.8%	Mar 22, 2029
NTRM	14090154	CC469551	990.9 PPM CARBON MONOXIDE/NITROGEN	$\pm$ 0.6%	Nov 15, 2025

ANALYTICAL EQUIPMENT		Last Multipoint Calibration
Instrument/Make/Model	Analytical Principle	
Nicolet 6550 AUP2010240 CO	FTIR	Oct 11, 2023
Nicolet 6550 AUP2010240 NO	FTIR	Oct 11, 2023
Nicolet 6550 AUP2010240 NO2	FTIR	Oct 11, 2023
Nicolet 6550 AUP2010240 SO2	FTIR	Oct 11, 2023

Triad Data Available Upon Request

NOTES: GROSS WEIGHT: 28.4 kg  
NET WEIGHT: 4.7 kg



Signature on file  
Approved for Release

MULTI-POINT GAS TEST REPORT


Test Date : Sep 20, 2024

Equipment : Gas Analyzer (NO<sub>2</sub>) Model : 42i  
Manufacturer : Thermo Scientific Serial Number : 1200636463

Standard Gas Concentration		Dilutor Detail	
Sulphur Dioxide (SO <sub>2</sub> )	42.89 PPM	Manufacturer :	Thermo Scientific
Nitric Oxide (NO)	46.77 PPM	Model :	146i
Methane (CH <sub>4</sub> )	- PPM	Serial Number :	1180540071
Carbon Monoxide (CO)	965.9		
Cylinder No. :	EB0159156		
Expiration Date :	Nov 6, 2026		

Multi-point gas test data

Reference Value (ppb)		Analyzer Display (ppb)	Difference Error	Percent Error	[% Error]
Level 1	Zero	0.0	0.00	0.00	0.00
Level 2	20.00%	100.0	100.7	0.70	0.70
Level 3	40.00%	200.0	200.5	0.25	0.25
Level 4	60.00%	300.0	300.9	0.30	0.30
Level 5	80.00%	400.0	400.0	0.00	0.00
Remark : Measuring Range		500.0 ppb	Average Difference (%)		
			:Acceptable Limit $\pm$ 5%		

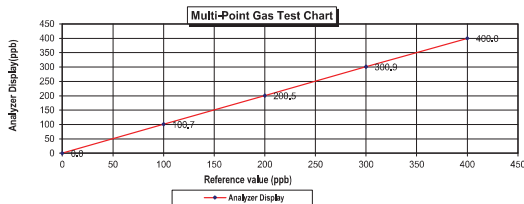

20 9 2567 20 Sep 2024

MULTI-POINT GAS TEST REPORT


Test Date : Sep 6, 2024

Equipment : Gas Analyzer (SO<sub>2</sub>) Model : 43i  
Manufacturer : Thermo SCIENTIFIC Serial Number : CM22387061

Standard Gas Concentration		Dilutor Detail	
Sulphur Dioxide (SO <sub>2</sub> )	42.89 PPM	Manufacturer :	Thermo SCIENTIFIC
Nitric Oxide (NO)	46.77 PPM	Model :	146i
Methane (CH <sub>4</sub> )	- PPM	Serial Number :	1180540071
Carbon Monoxide (CO)	965.9		
Cylinder No. :	EB0159156		
Expiration Date :	Nov 06, 2026		

Multi-point gas test data

Reference Value (ppb)		Analyzer Display (ppb)	Difference Error	Percent Error	[% Error]
Level 1	Zero	0.0	0.00	0.00	0.00
Level 2	20.00%	100.0	100.7	0.70	0.70
Level 3	40.00%	200.0	200.7	0.35	0.35
Level 4	60.00%	300.0	301.1	1.10	0.37
Level 5	80.00%	400.0	400.0	0.00	0.00
Remark : Measuring Range		500.0 ppb	Average Difference (%)		
			:Acceptable Limit $\pm$ 5%		

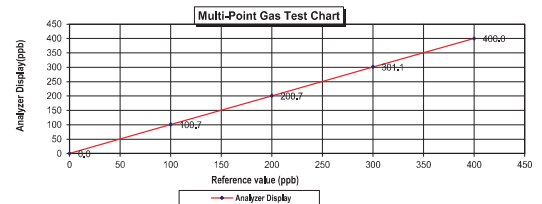

6 9 2567 6 Sep 2024

### MULTI-POINT GAS TEST REPORT


Test Date : June 19, 2024

Equipment : Gas Analyzer (SO<sub>2</sub>) Model : 43i  
Manufacturer : Thermo SCIENTIFIC Serial Number : CM22387063

Standard Gas Concentration			Dilutor Detail	
Sulphur Dioxide (SO <sub>2</sub> )	42.89	PPM	Manufacturer :	Thermo SCIENTIFIC
Nitric Oxide (NO)	46.77	PPM	Model :	146i
Methane (CH <sub>4</sub> )	-	PPM	Serial Number :	1180540071
Carbon Monoxide (CO)	965.9			
Cylinder No. :	EB01159156			
Expiration Date :	Nov 06, 2026			

#### Multi-point gas test data

Reference Value (ppb)			Analyzer Display (ppb)	Difference Error	Percent Error	[% Error ]
Level 1	Zero	0.0	0.0	0.00	0.00	0.00
Level 2	20.00%	100.0	100.8	0.80	0.79	0.79
Level 3	40.00%	200.0	200.7	0.70	0.35	0.35
Level 4	60.00%	300.0	301.1	1.10	0.37	0.37
Level 5	80.00%	400.0	400.0	0.00	0.00	0.00
Remark : Measuring Range 500.0 ppb			Average Difference (%)			0.30

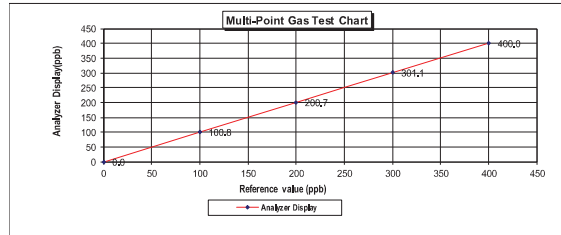

19/06/2567

19/June/2024

### MULTI-POINT GAS TEST REPORT


Test Date : Sep 6, 2024

Equipment : Gas Analyzer (SO<sub>2</sub>) Model : 43i  
Manufacturer : Thermo SCIENTIFIC Serial Number : CM22387066

Standard Gas Concentration			Dilutor Detail	
Sulphur Dioxide (SO <sub>2</sub> )	42.89	PPM	Manufacturer :	Thermo SCIENTIFIC
Nitric Oxide (NO)	46.77	PPM	Model :	146i
Methane (CH <sub>4</sub> )	-	PPM	Serial Number :	1180540071
Carbon Monoxide (CO)	965.9			
Cylinder No. :	EB01159156			
Expiration Date :	Nov 06, 2026			

#### Multi-point gas test data

	Reference Value (ppb)	Analyzer Display (ppb)	Difference Error	Percent Error	[% Error ]
Level 1	Zero	0.0	0.00	0.00	0.00
Level 2	20.00%	100.0	100.9	0.99	0.89
Level 3	40.00%	200.0	200.7	0.70	0.35
Level 4	60.00%	300.0	300.7	0.70	0.23
Level 5	80.00%	400.0	400.0	0.00	0.00
Remark : Measuring Range 500.0 ppb			Average Difference (%) 0.29		

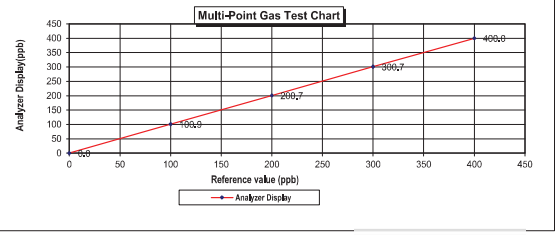

6/9/2567

6/Sep/2024

### MULTI-POINT GAS TEST REPORT


Test Date : Sep 6, 2024

Equipment : Gas Analyzer (SO<sub>2</sub>) Model : 43i  
Manufacturer : Thermo SCIENTIFIC Serial Number : CM22387065

Standard Gas Concentration			Dilutor Detail	
Sulphur Dioxide (SO <sub>2</sub> )	42.89	PPM	Manufacturer :	Thermo SCIENTIFIC
Nitric Oxide (NO)	46.77	PPM	Model :	146i
Methane (CH <sub>4</sub> )	-	PPM	Serial Number :	1180540071
Carbon Monoxide (CO)	965.9			
Cylinder No. :	EB01159156			
Expiration Date :	Nov 06, 2026			

#### Multi-point gas test data

	Reference Value (ppb)	Analyzer Display (ppb)	Difference Error	Percent Error	[% Error ]
Level 1	Zero	0.0	0.00	0.00	0.00
Level 2	20.00%	100.0	100.6	0.60	0.60
Level 3	40.00%	200.0	200.6	0.60	0.30
Level 4	60.00%	300.0	300.9	0.90	0.30
Level 5	80.00%	400.0	400.0	0.00	0.00
Remark : Measuring Range 500.0 ppb			Average Difference (%) 0.24		

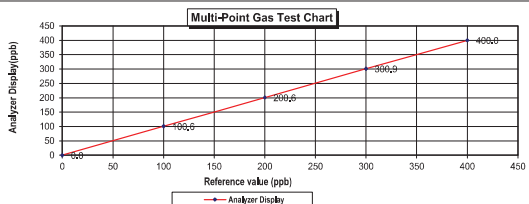

6/9/2567

6/Sep/2024

### MULTI-POINT GAS TEST REPORT


Test Date : May 15, 2024

Equipment : Gas Analyzer (SO<sub>2</sub>) Model : 43i  
Manufacturer : Thermo SCIENTIFIC Serial Number : CM22387067

Standard Gas Concentration			Dilutor Detail	
Sulphur Dioxide (SO <sub>2</sub> )	44.68	PPM	Manufacturer :	Thermo SCIENTIFIC
Nitric Oxide (NO)	45.94	PPM	Model :	146i
Methane (CH <sub>4</sub> )	-	PPM	Serial Number :	1180540071
Carbon Monoxide (CO)	984.8			
Cylinder No. :	EB0143262			
Expiration Date :	Jun 24, 2024			

#### Multi-point gas test data

	Reference Value (ppb)	Analyzer Display (ppb)	Difference Error	Percent Error	[% Error ]
Level 1	Zero	0.0	0.9	0.90	0.90
Level 2	20.00%	100.0	100.8	0.80	0.79
Level 3	40.00%	200.0	200.9	0.90	0.45
Level 4	60.00%	300.0	300.9	0.90	0.30
Level 5	80.00%	400.0	400.0	0.00	0.00
Remark : Measuring Range 500.0 ppb			Average Difference (%) 0.49		

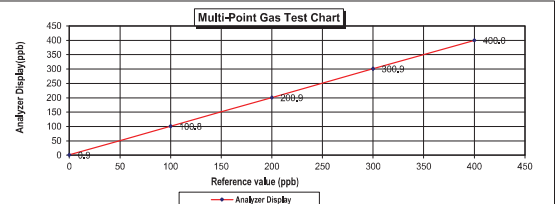

15/05/2567

15/May/2024


**MULTI-POINT GAS TEST REPORT**

Test Date : Sep 6, 2024

Equipment : Gas Analyzer (SO<sub>2</sub>) Model : 43i  
Manufacturer : Thermo SCIENTIFIC Serial Number : 1201778111

Standard Gas Concentration		Dilutor Detail	
Sulphur Dioxide (SO <sub>2</sub> )	42.89 PPM	Manufacturer :	Thermo SCIENTIFIC
Nitric Oxide (NO)	46.77 PPM	Model :	146i
Methane (CH <sub>4</sub> )	- PPM	Serial Number :	1180540071
Carbon Monoxide (CO)	965.9 PPM		
Cylinder No. :	EB01159156		
Expiration Date :	Nov 06, 2026		

Multi-point gas test data					
Level	Reference Value (ppb)	Analyzer Display (ppb)	Difference Error	Percent Error	[% Error]
Level 1	Zero	0.0	0.00	0.00	0.00
Level 2	20.00%	100.0	0.90	0.89	0.89
Level 3	40.00%	200.0	0.90	0.45	0.45
Level 4	60.00%	300.0	0.70	0.23	0.23
Level 5	80.00%	400.0	0.00	0.00	0.00
Remark : Measuring Range 500.0 ppb			Average Difference (%)		
:Acceptable Limit ± 5%			0.31		

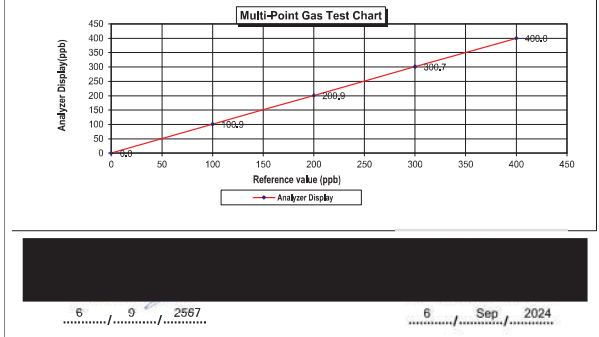


**MULTI-POINT GAS TEST REPORT**

Test Date : Sep 6, 2024

Equipment : Gas Analyzer (SO<sub>2</sub>) Model : 43i  
Manufacturer : Thermo SCIENTIFIC Serial Number : CM22387061

Standard Gas Concentration		Dilutor Detail	
Sulphur Dioxide (SO <sub>2</sub> )	42.89 PPM	Manufacturer :	Thermo SCIENTIFIC
Nitric Oxide (NO)	46.77 PPM	Model :	146i
Methane (CH <sub>4</sub> )	- PPM	Serial Number :	1180540071
Carbon Monoxide (CO)	965.9 PPM		
Cylinder No. :	EB01159156		
Expiration Date :	Nov 06, 2026		

Multi-point gas test data					
Level	Reference Value (ppb)	Analyzer Display (ppb)	Difference Error	Percent Error	[% Error]
Level 1	Zero	0.0	0.00	0.00	0.00
Level 2	20.00%	100.0	0.70	0.70	0.70
Level 3	40.00%	200.0	0.70	0.35	0.35
Level 4	60.00%	300.0	1.10	0.37	0.37
Level 5	80.00%	400.0	0.00	0.00	0.00
Remark : Measuring Range 500.0 ppb			Average Difference (%)		
:Acceptable Limit ± 5%			0.28		

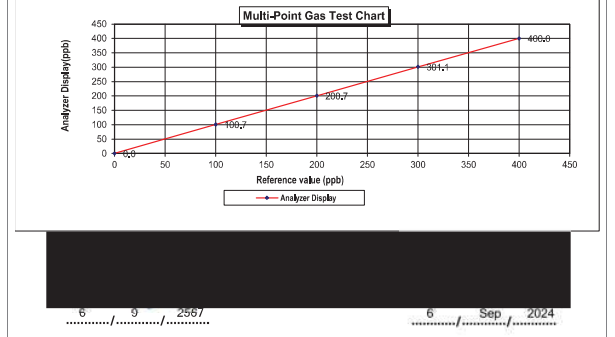

Airgas Specialty Gases  
Airgas USA LLC  
1500 United Drive  
Durham, NC 27713  
Airgas.com

## CERTIFICATE OF ANALYSIS

### Grade of Product: EPA PROTOCOL STANDARD

Customer: AIR LIQUIDE (THAILAND) LTD  
Part Number: E04NI99E15A01D3  
Cylinder Number: EB0159156  
Laboratory: 124 - Durham (SAP) - NC  
PGVP Number: B22023  
Gas Code: CO,NO,NOX,SO<sub>2</sub>,BALN

Reference Number: 122-402880224-1  
Cylinder Volume: 144.0 CF  
Cylinder Pressure: 2015 PSIG  
Valve Outlet: 660  
Certification Date: Nov 06, 2023  
Expiration Date: Nov 06, 2026

Certification performed in accordance with "EPA Traceability Protocol for Assay and Certification of Gaseous Calibration Standards (May 2012)" - current EPA 800R-12531, using the assay certificate (label). Analytical Microbiology does not require calibration for analytical reference. This cylinder has a 30M analytical uncertainty as stated below with a confidence level of 95%. There are no significant impurities which affect the use of this calibration mixture. All concentrations are on a mole/mole basis unless otherwise noted. The results relate only to the items tested. The report shall not be reproduced except in full without approval of the laboratory. Do not use this cylinder below 100 psig (i.e. 3.7 megapascals).

ANALYTICAL RESULTS					
Component	Requested Concentration	Actual Concentration	Protocol Method	Total Relative Uncertainty	Assay Dates
NOX	45.00 PPM	46.75 PPM	G1	±1.3% NIST Traceable	10/30/2023, 11/06/2023
NITRIC OXIDE	45.00 PPM	46.77 PPM	G1	±1.3% NIST Traceable	10/30/2023, 11/06/2023
SULFUR DIOXIDE	45.00 PPM	42.89 PPM	G1	±1.0% NIST Traceable	10/30/2023, 11/06/2023
CARBON MONOXIDE	1000 PPM	965.9 PPM	G1	±0.7% NIST Traceable	10/30/2023
NITROGEN	Balance				

CALIBRATION STANDARDS					
Type	Lot ID	Cylinder No	Concentration	Uncertainty	Expiration Date
NTRM	21060703	CC707554	48.41 PPM NITRIC OXIDE/NITROGEN	±1.2%	Sep 21, 2025
PRM		D913660	15.01 PPM NITROGEN DIOXIDE/AIR	±1.5%	Feb 18, 2023
GMIS	124206880	CC322689	4.873 PPM NITROGEN DIOXIDE/NITROGEN	±1.18%	Feb 17, 2026
NTRM	16061005	CC473180	49.02 PPM SULFUR DIOXIDE/NITROGEN	±0.8%	Mar 22, 2025
NTRM	14060154	CC436951	990.9 PPM CARBON MONOXIDE/NITROGEN	±1.06%	Nov 15, 2025

ANALYTICAL EQUIPMENT		
Instrument/Make/Model	Analytical Principle	Last Multipoint Calibration
Nicolet iSSO AUP2010249 CO	FTIR	Oct 11, 2023
Nicolet iSSO AUP2010249 NO	FTIR	Oct 11, 2023
Nicolet iSSO AUP2010249 NO2	FTIR	Oct 11, 2023
Nicolet iSSO AUP2010249 SO2	FTIR	Oct 11, 2023

Triad Data Available Upon Request

NOTES: GROSS WEIGHT: 28.4 kg  
NET WEIGHT: 4.7 kg



Signature on file  
Approved for Release


**MULTI-POINT GAS TEST REPORT**

Test Date : June 19, 2024

Equipment : Gas Analyzer (SO<sub>2</sub>) Model : 43i  
Manufacturer : Thermo SCIENTIFIC Serial Number : CM22387063

Standard Gas Concentration		Dilutor Detail	
Sulphur Dioxide (SO <sub>2</sub> )	42.89 PPM	Manufacturer :	Thermo SCIENTIFIC
Nitric Oxide (NO)	46.77 PPM	Model :	146i
Methane (CH <sub>4</sub> )	- PPM	Serial Number :	1180540071
Carbon Monoxide (CO)	965.9 PPM		
Cylinder No. :	EB0159156		
Expiration Date :	Nov 06, 2026		

Multi-point gas test data					
Level	Reference Value (ppb)	Analyzer Display (ppb)	Difference Error	Percent Error	[% Error]
Level 1	Zero	0.0	0.00	0.00	0.00
Level 2	20.00%	100.0	0.80	0.79	0.79
Level 3	40.00%	200.0	0.70	0.35	0.35
Level 4	60.00%	300.0	1.10	0.37	0.37
Level 5	80.00%	400.0	0.00	0.00	0.00
Remark : Measuring Range 500.0 ppb			Average Difference (%)		
:Acceptable Limit ± 5%			0.30		

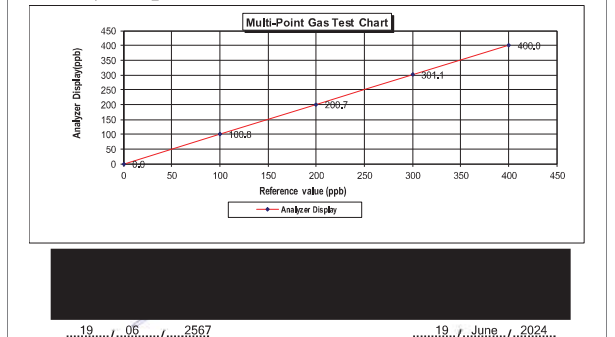

MULTI-POINT GAS TEST REPORT


Test Date : Sep 6, 2024

Equipment : Gas Analyzer (SO<sub>2</sub>) Model : 43i  
Manufacturer : Thermo SCIENTIFIC Serial Number : CM22387065

Standard Gas Concentration			Dilutor Detail	
Sulphur Dioxide (SO <sub>2</sub> )	42.89	PPM	Manufacturer :	Thermo SCIENTIFIC
Nitric Oxide (NO)	46.77	PPM	Model :	146i
Methane (CH <sub>4</sub> )	-	PPM	Serial Number :	1180540071
Carbon Monoxide (CO)	965.9			
Cylinder No. :	EB01159156			
Expiration Date :	Nov 06, 2026			

Multi-point gas test data

	Reference Value (ppb)		Analyzer Display (ppb)	Difference Error	Percent Error	[% Error ]
Level 1	Zero	0.0	0.0	0.00	0.00	0.00
Level 2	20.00%	100.0	100.6	0.60	0.60	0.60
Level 3	40.00%	200.0	200.6	0.60	0.30	0.30
Level 4	60.00%	300.0	300.9	0.90	0.30	0.30
Level 5	80.00%	400.0	400.0	0.00	0.00	0.00
Remark : Measuring Range 500.0 ppb			Average Difference (%)			
:Acceptable Limit $\pm$ 5%			0.24			

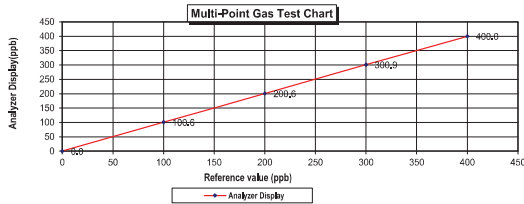

6 9 2567 6 Sep 2024

MULTI-POINT GAS TEST REPORT


Test Date : May 15, 2024

Equipment : Gas Analyzer (SO<sub>2</sub>) Model : 43i  
Manufacturer : Thermo SCIENTIFIC Serial Number : CM22387067

Standard Gas Concentration			Dilutor Detail	
Sulphur Dioxide (SO <sub>2</sub> )	44.68	PPM	Manufacturer :	Thermo SCIENTIFIC
Nitric Oxide (NO)	45.94	PPM	Model :	146i
Methane (CH <sub>4</sub> )	-	PPM	Serial Number :	1180540071
Carbon Monoxide (CO)	984.8			
Cylinder No. :	EB0143262			
Expiration Date :	Jun 24, 2024			

Multi-point gas test data

	Reference Value (ppb)		Analyzer Display (ppb)	Difference Error	Percent Error	[% Error ]
Level 1	Zero	0.0	0.9	0.90	0.90	0.90
Level 2	20.00%	100.0	100.8	0.80	0.79	0.79
Level 3	40.00%	200.0	200.9	0.90	0.45	0.45
Level 4	60.00%	300.0	300.9	0.90	0.30	0.30
Level 5	80.00%	400.0	400.0	0.00	0.00	0.00
Remark : Measuring Range 500.0 ppb			Average Difference (%)			
:Acceptable Limit $\pm$ 5%			0.49			

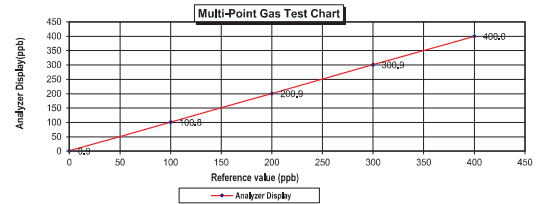

15 05 2567 15 May 2024

MULTI-POINT GAS TEST REPORT


Test Date : Sep 6, 2024

Equipment : Gas Analyzer (SO<sub>2</sub>) Model : 43i  
Manufacturer : Thermo SCIENTIFIC Serial Number : CM22387066

Standard Gas Concentration			Dilutor Detail	
Sulphur Dioxide (SO <sub>2</sub> )	42.89	PPM	Manufacturer :	Thermo SCIENTIFIC
Nitric Oxide (NO)	46.77	PPM	Model :	146i
Methane (CH <sub>4</sub> )	-	PPM	Serial Number :	1180540071
Carbon Monoxide (CO)	965.9			
Cylinder No. :	EB01159156			
Expiration Date :	Nov 06, 2026			

Multi-point gas test data

	Reference Value (ppb)		Analyzer Display (ppb)	Difference Error	Percent Error	[% Error ]
Level 1	Zero	0.0	0.0	0.00	0.00	0.00
Level 2	20.00%	100.0	100.9	0.90	0.89	0.89
Level 3	40.00%	200.0	200.7	0.70	0.35	0.35
Level 4	60.00%	300.0	300.7	0.70	0.23	0.23
Level 5	80.00%	400.0	400.0	0.00	0.00	0.00
Remark : Measuring Range 500.0 ppb			Average Difference (%)			
:Acceptable Limit $\pm$ 5%			0.29			

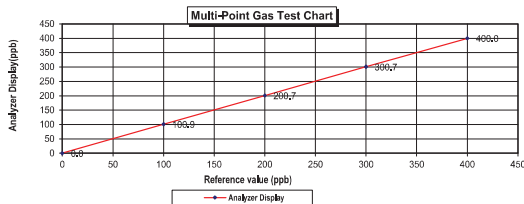

6 9 2567 6 Sep 2024

MULTI-POINT GAS TEST REPORT


Test Date : Sep 6, 2024

Equipment : Gas Analyzer (SO<sub>2</sub>) Model : 43i  
Manufacturer : Thermo SCIENTIFIC Serial Number : 1201778111

Standard Gas Concentration			Dilutor Detail	
Sulphur Dioxide (SO <sub>2</sub> )	42.89	PPM	Manufacturer :	Thermo SCIENTIFIC
Nitric Oxide (NO)	46.77	PPM	Model :	146i
Methane (CH <sub>4</sub> )	-	PPM	Serial Number :	1180540071
Carbon Monoxide (CO)	965.9			
Cylinder No. :	EB01159156			
Expiration Date :	Nov 06, 2026			

Multi-point gas test data

	Reference Value (ppb)		Analyzer Display (ppb)	Difference Error	Percent Error	[% Error ]
Level 1	Zero	0.0	0.0	0.00	0.00	0.00
Level 2	20.00%	100.0	100.9	0.90	0.89	0.89
Level 3	40.00%	200.0	200.9	0.90	0.45	0.45
Level 4	60.00%	300.0	300.7	0.70	0.23	0.23
Level 5	80.00%	400.0	400.0	0.00	0.00	0.00
Remark : Measuring Range 500.0 ppb			Average Difference (%)			
:Acceptable Limit $\pm$ 5%			0.31			

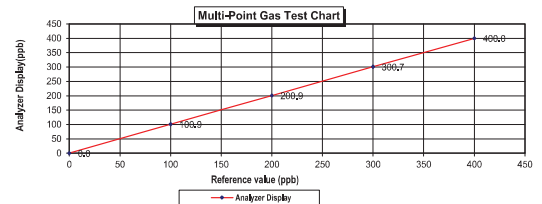

6 9 2567 6 Sep 2024

## CERTIFICATE OF ANALYSIS

### Grade of Product: EPA PROTOCOL STANDARD

Customer: AIR LIQUIDE  
(THAILAND) LTD  
Part Number: E04N199E15A01D3  
Cylinder Number: EB0159156  
Laboratory: 124 - Durham (SAP) - NC  
PGVP Number: B22023  
Gas Code: CO,NO,NOX,SO2,BALN  
Reference Number: 122-402880224-1  
Cylinder Volume: 144.0 CF  
Cylinder Pressure: 2015 PSIG  
Valve Outlet: 660  
Certification Date: Nov 06, 2023  
Expiration Date: Nov 06, 2026

Certification performed in accordance with "EPA Traceability Protocol for Assay and Certification of Gaseous Calibration Standards (May 2017)" (www.epa.gov/900R-12531), using the assay procedures listed. Analytical Metrology does not require certification for analytical interference. This cylinder has a total analytical uncertainty as stated below with a confidence level of 95%. There are no significant impurities which affect the use of this calibration mixture. All concentrations are on a mole/mole basis unless otherwise noted. The results relate only to the items tested. The report shall not be reproduced except in full without approval of the laboratory. Do Not Use This Cylinder below 100 psig, i.e. 0.7 megapascals.

ANALYTICAL RESULTS					
Component	Requested Concentration	Actual Concentration	Protocol Method	Total Relative Uncertainty	Assay Dates
NOX	45.00 PPM	46.78 PPM	G1	+/- 1.3% NIST Traceable	10/30/2023, 11/06/2023
NITRIC OXIDE	45.00 PPM	46.77 PPM	G1	+/- 1.3% NIST Traceable	10/30/2023, 11/06/2023
SULFUR DIOXIDE	45.00 PPM	42.89 PPM	G1	+/- 1.0% NIST Traceable	10/30/2023, 11/06/2023
CARBON MONOXIDE	1000 PPM	965.9 PPM	G1	+/- 0.7% NIST Traceable	10/30/2023
NITROGEN	Balance				

CALIBRATION STANDARDS					
Type	Lot ID	Cylinder No	Concentration	Uncertainty	Expiration Date
NTRM	21080703	CC707954	48.41 PPM NITRIC OXIDE/NITROGEN	+/- 1.2%	Sep 21, 2025
PRM	PRM	D913660	15.01 PPM NITROGEN DIOXIDE/AIR	+/- 1.8%	Feb 18, 2023
GMS	124208889	CC222689	4.573 PPM NITROGEN DIOXIDE/NITROGEN	+/- 1.8%	Feb 17, 2026
NTRM	16081005	CC473180	49.02 PPM SULFUR DIOXIDE/NITROGEN	+/- 0.8%	Mar 22, 2028
NTRM	14060154	CC436951	990.9 PPM CARBON MONOXIDE/NITROGEN	+/- 0.6%	Nov 15, 2025

ANALYTICAL EQUIPMENT		
Instrument/Make/Model	Analytical Principle	Last Multipoint Calibration
Nicolet 650 AUP2010240 CO	FTIR	Oct 11, 2023
Nicolet 650 AUP2010249 NO	FTIR	Oct 11, 2023
Nicolet 650 AUP2010249 NO2	FTIR	Oct 11, 2023
Nicolet 650 AUP2010249 SO2	FTIR	Oct 11, 2023

Triad Data Available Upon Request

NOTES: GROSS WEIGHT: 28.4 kg  
NET WEIGHT: 4.7 kg



Signature on file

Approved for Release

ภาคผนวก จ

---

หนังสืออนุญาตขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน

ที่ อภ ๐๓๑๐(๑)/ ๑๘๗ ๕



กรมโรงงานอุตสาหกรรม  
ถนนพระรามที่ ๖ แขวงทุ่งพญาไท  
เขตราชเทวี กรุงเทพฯ ๑๐๔๐๐

๐ ๙ กุมภาพันธ์ ๒๕๖๕

เรื่อง ต่ออายุหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน

เรียน กรรมการผู้จัดการ บริษัท ยูโนเด็ค แอนนาลิสต์ แอนด์ เอ็นจิเนียริ่ง คอนซัลแตนท์ จำกัด

อ้างถึง คำขอขึ้นทะเบียน/ต่ออายุ/เปลี่ยนแปลงบุคลากร และชนิดสารมลพิษของห้องปฏิบัติการวิเคราะห์เอกชน ลงวันที่ ๒๗ ธันวาคม ๒๕๖๔

- สิ่งที่ส่งมาด้วย ๑. รายชื่อผู้ควบคุมดูแลห้องปฏิบัติการวิเคราะห์ จำนวน ๔๐ ราย  
๒. รายชื่อเจ้าหน้าที่ประจำห้องปฏิบัติการวิเคราะห์ จำนวน ๑๐๖ ราย  
๓. ขอบข่ายสารมลพิษที่ได้รับขึ้นทะเบียนจากกรมโรงงานอุตสาหกรรม

ตามหนังสือที่ยังอ้างถึง บริษัท ยูโนเด็ค แอนนาลิสต์ แอนด์ เอ็นจิเนียริ่ง คอนซัลแตนท์ จำกัด ขอต่ออายุหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน เลขทะเบียน ๖-๑๔๕ สถานที่ตั้งเลขที่ ๓ ซอยอุดมสุข ๔๑ ถนนสุขุมวิท แขวงบางจาก เขตพระโขนง กรุงเทพมหานคร ต่อกรมโรงงานอุตสาหกรรม นั้น

กรมโรงงานอุตสาหกรรมพิจารณาแล้ว ให้บริษัท ยูโนเด็ค แอนนาลิสต์ แอนด์ เอ็นจิเนียริ่ง คอนซัลแตนท์ จำกัด ต่ออายุหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน โดยมีองค์ประกอบดังนี้  
ก. ผู้ควบคุมดูแลห้องปฏิบัติการวิเคราะห์ จำนวน ๔๐ ราย ตามสิ่งที่ส่งมาด้วย ๑  
ข. เจ้าหน้าที่ประจำห้องปฏิบัติการวิเคราะห์ จำนวน ๑๐๖ ราย ตามสิ่งที่ส่งมาด้วย ๒  
ค. ขอบข่ายสารมลพิษที่ได้รับขึ้นทะเบียนให้วิเคราะห์ในน้ำเสีย น้ำใต้ดิน อากาศเสีย สิ่งปฏิกูล หรือวัสดุที่ไม่ใช้แล้ว และดิน ตามสิ่งที่ส่งมาด้วย ๓

หนังสือฉบับนี้จะหมดอายุในวันที่ ๒ กุมภาพันธ์ ๒๕๖๘ หากประสงค์จะต่ออายุหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน ให้ยื่นคำขอต่ออายุพร้อมเอกสารประกอบคำขอต่อกรมโรงงานอุตสาหกรรมภายใน ๓๐ วัน ก่อนวันสิ้นสุดของหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน ทั้งนี้ สามารถยื่นคำขอผ่านระบบอิเล็กทรอนิกส์ได้ทั้งหน้าเว็บไซต์กรมโรงงานอุตสาหกรรม ตาม QR Code ที่แนบมาด้วย

จึงเรียนมาเพื่อทราบ

ขอแสดงความนับถือ



ผู้อำนวยการกองประเมินและขึ้นทะเบียนโรงงาน  
ปฏิบัติการทางเคมีและชีวเคมี กรมโรงงานอุตสาหกรรม



ยื่นคำขอผ่านระบบอิเล็กทรอนิกส์

กองวิจัยและเตือนภัยมลพิษโรงงาน

กลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษและทะเบียนห้องปฏิบัติการ

โทร. ๐ ๒๕๓๐ ๖๓๑๒ ต่อ ๒๑๐๓-๕

โทรสาร ๐ ๒๕๓๐ ๖๓๑๒ ต่อ ๒๑๕๕

ไปรษณีย์อิเล็กทรอนิกส์ sarabang@dlw.gmail.go.th

สิ่งที่ส่งมาด้วย ๑

เอกสารแนบท้ายหนังสือรับต่ออายุขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน  
บริษัท ยูโนเด็ค แอนนาลิสต์ แอนด์ เอ็นจิเนียริ่ง คอนซัลแตนท์ จำกัด เลขทะเบียน ๖-๑๔๕  
ที่ อภ ๐๓๑๐(๑)/ ๑๘๗ ๕ ลงวันที่ ๐ ๙ กุมภาพันธ์ ๒๕๖๕

ก. ผู้ควบคุมดูแลห้องปฏิบัติการวิเคราะห์ จำนวน ๔๐ ราย

- ๑)
- ๒)
- ๓)
- ๔)
- ๕)
- ๖)
- ๗)
- ๘)
- ๙)
- ๑๐)
- ๑๑)
- ๑๒)
- ๑๓)
- ๑๔)
- ๑๕)
- ๑๖)
- ๑๗)
- ๑๘)
- ๑๙)
- ๒๐)
- ๒๑)
- ๒๒)
- ๒๓)
- ๒๔)
- ๒๕)
- ๒๖)
- ๒๗)
- ๒๘)
- ๒๙)
- ๓๐)
- ๓๑)
- ๓๒)
- ๓๓)
- ๓๔)
- ๓๕)

ผู้อำนวยการกองประเมินและขึ้นทะเบียนโรงงาน  
ปฏิบัติการทางเคมีและชีวเคมี กรมโรงงานอุตสาหกรรม

๓๖) นายสุมนีรัฐ...

-๒-

- ๓๖)
- ๓๗)
- ๓๘)
- ๓๙)
- ๔๐)



ผู้อำนวยการกองประเมินและขึ้นทะเบียนโรงงาน  
ปฏิบัติการทางเคมีและชีวเคมี กรมโรงงานอุตสาหกรรม

สิ่งที่ส่งมาด้วย ๒

เอกสารแนบท้ายหนังสือรับต่ออายุขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน  
บริษัท ยูโนเด็ค แอนนาลิสต์ แอนด์ เอ็นจิเนียริ่ง คอนซัลแตนท์ จำกัด เลขทะเบียน ๖-๑๔๕  
ที่ อภ ๐๓๑๐(๑)/ ๑๘๗ ๕ ลงวันที่ ๐ ๙ กุมภาพันธ์ ๒๕๖๕

ข. เจ้าหน้าที่ประจำห้องปฏิบัติการวิเคราะห์ จำนวน ๑๐๖ ราย

- ๑)
- ๒)
- ๓)
- ๔)
- ๕)
- ๖)
- ๗)
- ๘)
- ๙)
- ๑๐)
- ๑๑)
- ๑๒)
- ๑๓)
- ๑๔)
- ๑๕)
- ๑๖)
- ๑๗)
- ๑๘)
- ๑๙)
- ๒๐)
- ๒๑)
- ๒๒)
- ๒๓)
- ๒๔)
- ๒๕)
- ๒๖)
- ๒๗)
- ๒๘)
- ๒๙)
- ๓๐)
- ๓๑)
- ๓๒)
- ๓๓)
- ๓๔)
- ๓๕)

ผู้อำนวยการกองประเมินและขึ้นทะเบียนโรงงาน  
ปฏิบัติการทางเคมีและชีวเคมี กรมโรงงานอุตสาหกรรม

๓๖) นายสมานันท์...



๓๖) นายอรรถวิทย์พงษ์...

ผู้ช่วยศาสตราจารย์และคณบดีคณะวิศวกรรมศาสตร์  
ปฏิจิราคารามณชฌิมคัมภีร์มหาวิทยาลัยราชภัฏวราวุฒ



ผู้ช่วยศาสตราจารย์และคณบดีคณะวิศวกรรมศาสตร์  
ปฏิจิราคารามณชฌิมคัมภีร์มหาวิทยาลัยราชภัฏวราวุฒ

สิ่งที่ส่งมาด้วย ๓

เอกสารแนบท้ายหนังสือรับต่ออาชญากรรมขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกสาร  
บริษัท ยูนิเทค แอนนาลิสต์ แอนด์ เอ็นจิเนียริง คอนซัลแตนท์ จำกัด เลขทะเบียน ๖-๑๕๕  
ที่ อภ ๐๓๑๐(๑)/ ๑๘๗๕ ลงวันที่ ๐๙ กุมภาพันธ์ ๒๕๖๕

ขอขยายสารมลพิษที่ได้รับขึ้นทะเบียนจากกรมโรงงานอุตสาหกรรม จำนวน ๑๕๗ รายการ

แนบรายชื่อ จำนวน 46 รายการ

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
1	Aldrin	Liquid-Liquid Extraction, Gas Chromatographic Method <sup>(4)</sup>
2	Arsenic	1) Digestion, Hydride Generation/Atomic Absorption Spectrometric Method <sup>(4)</sup> 2) Digestion, Inductively Coupled Plasma Method <sup>(4)</sup>
3	Barium	Digestion, Inductively Coupled Plasma Method <sup>(4)</sup>
4	α-BHC	Liquid-Liquid Extraction, Gas Chromatographic Method <sup>(4)</sup>
5	β-BHC	Liquid-Liquid Extraction, Gas Chromatographic Method <sup>(4)</sup>
6	δ-BHC	Liquid-Liquid Extraction, Gas Chromatographic Method <sup>(4)</sup>
7	γ-BHC	Liquid-Liquid Extraction, Gas Chromatographic Method <sup>(4)</sup>
8	Biochemical Oxygen Demand	1) 5-Day BOD Test, Azide Modification Method <sup>(4)</sup> 2) 5-Day BOD Test, Membrane Electrode Method <sup>(4)</sup>
9	Cadmium	1) Digestion, Direct Air-Acetylene Flame Method <sup>(4)</sup> 2) Digestion, Electrothermal Atomic Absorption Spectrometric Method <sup>(4)</sup> 3) Digestion, Inductively Coupled Plasma Method <sup>(4)</sup>
10	Chemical Oxygen Demand	1) Closed Reflux, Titrimetric Method <sup>(4)</sup> 2) Closed Reflux, Colorimetric Method <sup>(4)</sup> 3) Open Reflux, Titrimetric Method <sup>(4)</sup>
11	Chlordane	Liquid-Liquid Extraction, Gas Chromatographic Method <sup>(4)</sup>
12	Chromium	1) Digestion, Direct Air-Acetylene Flame Method <sup>(4)</sup> 2) Digestion, Electrothermal Atomic Absorption Spectrometric Method <sup>(4)</sup> 3) Digestion, Inductively Coupled Plasma Method <sup>(4)</sup>
13	Color	ADMI Weighted-Ordinate Spectrophotometric Method <sup>(4)</sup>
14	Copper	1) Digestion, Direct Air-Acetylene Flame Method <sup>(4)</sup> 2) Digestion, Electrothermal Atomic Absorption Spectrometric Method <sup>(4)</sup> 3) Digestion, Inductively Coupled Plasma Method <sup>(4)</sup>
15	Cyanide	1) Distillation, Colorimetric Method <sup>(4)</sup> 2) Flow Injection Analysis Method <sup>(4)</sup>

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
16	o,p'-DDT	Liquid-Liquid Extraction, Gas Chromatographic Method <sup>(4)</sup>
17	4,4'-DDD	Liquid-Liquid Extraction, Gas Chromatographic Method <sup>(4)</sup>
18	4,4'-DDE	Liquid-Liquid Extraction, Gas Chromatographic Method <sup>(4)</sup>
19	4,4'-DDT	Liquid-Liquid Extraction, Gas Chromatographic Method <sup>(4)</sup>
20	Dieldrin	Liquid-Liquid Extraction, Gas Chromatographic Method <sup>(4)</sup>
21	Endosulfan I	Liquid-Liquid Extraction, Gas Chromatographic Method <sup>(4)</sup>
22	Endosulfan II	Liquid-Liquid Extraction, Gas Chromatographic Method <sup>(4)</sup>
23	Endosulfan sulfate	Liquid-Liquid Extraction, Gas Chromatographic Method <sup>(4)</sup>
24	Endrin	Liquid-Liquid Extraction, Gas Chromatographic Method <sup>(4)</sup>
25	Endrin aldehyde	Liquid-Liquid Extraction, Gas Chromatographic Method <sup>(4)</sup>
26	Formaldehyde	Distillation, Colorimetric Method <sup>(4)</sup>
27	Free Chlorine	1) Iodometric Method <sup>(4)</sup> 2) DPD Ferrous Titrimetric Method <sup>(4)</sup>
28	Heptachlor	Liquid-Liquid Extraction, Gas Chromatographic Method <sup>(4)</sup>
29	Heptachlor Epoxide	Liquid-Liquid Extraction, Gas Chromatographic Method <sup>(4)</sup>
30	Hexavalent Chromium	1) Colorimetric Method <sup>(4)</sup> 2) Extraction, Direct Air-Acetylene Flame Method <sup>(4)</sup>
31	Lead	1) Digestion, Direct Air-Acetylene Flame Method <sup>(4)</sup> 2) Digestion, Electrothermal Atomic Absorption Spectrometric Method <sup>(4)</sup> 3) Digestion, Inductively Coupled Plasma Method <sup>(4)</sup>
32	Manganese	1) Digestion, Direct Air-Acetylene Flame Method <sup>(4)</sup> 2) Digestion, Electrothermal Atomic Absorption Spectrometric Method <sup>(4)</sup> 3) Digestion, Inductively Coupled Plasma Method <sup>(4)</sup>
33	Mercury	Digestion, Cold-Vapor Atomic Absorption Spectrometric Method <sup>(4)</sup>
34	Methoxychlor	Liquid-Liquid Extraction, Gas Chromatographic Method <sup>(4)</sup>
35	Nickel	1) Digestion, Direct Air-Acetylene Flame Method <sup>(4)</sup> 2) Digestion, Electrothermal Atomic Absorption Spectrometric Method <sup>(4)</sup> 3) Digestion, Inductively Coupled Plasma Method <sup>(4)</sup>

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
36	Oil & Grease	1) Liquid-Liquid, Partition-Gravimetric Method <sup>(4)</sup> 2) Soxhlet Extraction Method <sup>(4)</sup>
37	pH	Electrometric Method <sup>(4)</sup>
38	Phenols	1) Distillation, Chloroform Extraction Method <sup>(4)</sup> 2) Distillation, Direct Photometric Method <sup>(4)</sup>
39	Selenium	1) Digestion, Hydride Generation/Atomic Absorption Spectrometric Method <sup>(4)</sup> 2) Digestion, Inductively Coupled Plasma Method <sup>(4)</sup>
40	Sulfide	1) Iodometric Method <sup>(4)</sup> 2) Methylene Blue Method <sup>(4)</sup>
41	Temperature	Laboratory and Field Methods <sup>(4)</sup>
42	Total Dissolved Solids	Dried at 180 °C <sup>(4)</sup>
43	Total Kjeldahl Nitrogen	Semi-Micro-Kjeldahl Method <sup>(4)</sup>
44	Total Suspended Solids	Dried at 103-105 °C <sup>(4)</sup>
45	Trivalent Chromium	1) Digestion, Direct Air-Acetylene Flame Method; Colorimetric Method; Calculation <sup>(4)</sup> 2) Digestion, Inductively Coupled Plasma Method; Colorimetric Method; Calculation <sup>(4)</sup>
46	Zinc	1) Digestion, Direct Air-Acetylene Flame Method <sup>(4)</sup> 2) Digestion, Electrothermal Atomic Absorption Spectrometric Method <sup>(4)</sup> 3) Digestion, Inductively Coupled Plasma Method <sup>(4)</sup>

น้ำใต้ดิน จำนวน 126 รายการ

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
1	Acenaphthene	1) Liquid-Liquid Extraction, Gas Chromatographic Method <sup>(4)</sup> 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>(4)</sup>
2	Acetone	Purge and Trap Gas Chromatographic/Mass Spectrometric Method <sup>(4)</sup>
3	Aldrin	1) Liquid-Liquid Extraction, Gas Chromatographic Method <sup>(4)</sup> 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>(4)</sup> <i>ดูภาพ</i>

4 Anthracene...

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
4	Anthracene	1) Liquid-Liquid Extraction, Gas Chromatographic Method <sup>(4)</sup> 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>(4)</sup>
5	Antimony	Digestion, Inductively Coupled Plasma Method <sup>(4)</sup>
6	Arsenic	1) Digestion, Hydride Generation/Atomic Absorption Spectrometric Method <sup>(4)</sup> 2) Digestion, Inductively Coupled Plasma Method <sup>(4)</sup>
7	Atrazine	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>(4)</sup>
8	Barium	1) Digestion, Electrothermal Atomic Absorption Spectrometric Method <sup>(4)</sup> 2) Digestion, Inductively Coupled Plasma Method <sup>(4)</sup>
9	Benz(a)anthracene	1) Liquid-Liquid Extraction, Gas Chromatographic Method <sup>(4)</sup> 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>(4)</sup>
10	Benzene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method <sup>(4)</sup>
11	Benzo(b)fluoranthene	1) Liquid-Liquid Extraction, Gas Chromatographic Method <sup>(4)</sup> 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>(4)</sup>
12	Benzo(k)fluoranthene	1) Liquid-Liquid Extraction, Gas Chromatographic Method <sup>(4)</sup> 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>(4)</sup>
13	Benzoic acid	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>(4)</sup>
14	Benzo(a)pyrene	1) Liquid-Liquid Extraction, Gas Chromatographic Method <sup>(4)</sup> 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>(4)</sup> <i>ดูภาพ</i>

15 Benzo(g,h,i)perylene...

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
15	Benzo(g,h,i)perylene	1) Liquid-Liquid Extraction, Gas Chromatographic Method <sup>(4)</sup> 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>(4)</sup>
16	Beryllium	Digestion, Inductively Coupled Plasma Method <sup>(4)</sup>
17	Bis(2-chloroethyl)ether	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>(4)</sup>
18	Bis(2-ethylhexyl)phthalate	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>(4)</sup>
19	Bromodichloromethane	Purge and Trap Gas Chromatographic/Mass Spectrometric Method <sup>(4)</sup>
20	Bromoform	Purge and Trap Gas Chromatographic/Mass Spectrometric Method <sup>(4)</sup>
21	Butanol	Purge and Trap Gas Chromatographic/Mass Spectrometric Method <sup>(4)</sup>
22	Butyl benzyl phthalate	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>(4)</sup>
23	Cadmium	1) Digestion, Direct Air-Acetylene Flame Method <sup>(4)</sup> 2) Digestion, Electrothermal Atomic Absorption Spectrometric Method <sup>(4)</sup> 3) Digestion, Inductively Coupled Plasma Method <sup>(4)</sup>
24	Carbazole	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>(4)</sup>
25	Carbon disulfide	Purge and Trap Gas Chromatographic/Mass Spectrometric Method <sup>(4)</sup>
26	Carbon tetrachloride	Purge and Trap Gas Chromatographic/Mass Spectrometric Method <sup>(4)</sup>
27	Chlordane	1) Liquid-Liquid Extraction, Gas Chromatographic Method <sup>(4)</sup> 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>(4)</sup>
28	p-Chloroaniline	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>(4)</sup>
29	Chlorobenzene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method <sup>(4)</sup> <i>ดูภาพ</i>

30 Chlorodibromomethane...

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
30	Chlorodibromomethane	Purge and Trap Gas Chromatographic/Mass Spectrometric Method <sup>(4)</sup>
31	Chloroform	Purge and Trap Gas Chromatographic/Mass Spectrometric Method <sup>(4)</sup>
32	2-Chlorophenol	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>(4)</sup>
33	Chromium	1) Digestion, Direct Air-Acetylene Flame Method <sup>(4)</sup> 2) Digestion, Electrothermal Atomic Absorption Spectrometric Method <sup>(4)</sup> 3) Digestion, Inductively Coupled Plasma Method <sup>(4)</sup>
34	Chromium (III)	1) Digestion, Direct Air-Acetylene Flame Method; Colorimetric Method; Calculation <sup>(4)</sup> 2) Digestion, Inductively Coupled Plasma Method; Colorimetric Method; Calculation <sup>(4)</sup>
35	Chromium (VI)	1) Colorimetric Method <sup>(4)</sup> 2) Extraction, Air-Acetylene Flame Method <sup>(4)</sup>
36	Chrysene	1) Liquid-Liquid Extraction, Gas Chromatographic Method <sup>(4)</sup> 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>(4)</sup>
37	Cyanide	Distillation, Colorimetric Method <sup>(4)</sup>
38	2,4-D	Liquid-Liquid Extraction, Gas Chromatographic Method <sup>(4)</sup>
39	DDD	1) Liquid-Liquid Extraction, Gas Chromatographic Method <sup>(4)</sup> 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>(4)</sup>
40	DDE	1) Liquid-Liquid Extraction, Gas Chromatographic Method <sup>(4)</sup> 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>(4)</sup>
41	DDT	1) Liquid-Liquid Extraction, Gas Chromatographic Method <sup>(4)</sup> 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>(4)</sup> <i>ดูภาพ</i>

42 Dibenz(a,h)anthracene...

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
42	Dibenz(a,h)anthracene	1) Liquid-Liquid Extraction, Gas Chromatographic Method <sup>(4)</sup> 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>(4)</sup>
43	Di-n-butyl phthalate	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>(4)</sup>
44	1,2-Dichlorobenzene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method <sup>(4)</sup>
45	1,3-Dichlorobenzene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method <sup>(4)</sup>
46	1,4-Dichlorobenzene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method <sup>(4)</sup>
47	3,3'-Dichlorobenzidine	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>(4)</sup>
48	1,1-Dichloroethane	Purge and Trap Gas Chromatographic/Mass Spectrometric Method <sup>(4)</sup>
49	1,2-Dichloroethane	Purge and Trap Gas Chromatographic/Mass Spectrometric Method <sup>(4)</sup>
50	1,1-Dichloroethylene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method <sup>(4)</sup>
51	cis-1,2-Dichloroethylene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method <sup>(4)</sup>
52	trans-1,2-Dichloroethylene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method <sup>(4)</sup>
53	2,4-Dichlorophenol	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>(4)</sup>
54	1,2-Dichloropropene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method <sup>(4)</sup>
55	1,3-Dichloropropane	Purge and Trap Gas Chromatographic/Mass Spectrometric Method <sup>(4)</sup>
56	1,3-Dichloropropene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method <sup>(4)</sup>
57	Dieldrin	1) Liquid-Liquid Extraction, Gas Chromatographic Method <sup>(4)</sup> 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>(4)</sup>

58 Diethyl phthalate...

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
58	Diethyl phthalate	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>(4)</sup>
59	2,4-Dimethylphenol	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>(4)</sup>
60	2,4-Dinitrophenol	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>(4)</sup>
61	2,4-Dinitrotoluene	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>(4)</sup>
62	2,6-Dinitrotoluene	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>(4)</sup>
63	Di-n-Octyl phthalate	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>(4)</sup>
64	Endosulfan	1) Liquid-Liquid Extraction, Gas Chromatographic Method <sup>(4)</sup> 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>(4)</sup>
65	Endrin	1) Liquid-Liquid Extraction, Gas Chromatographic Method <sup>(4)</sup> 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>(4)</sup>
66	Ethylbenzene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method <sup>(4)</sup>
67	Fluoranthene	1) Liquid-Liquid Extraction, Gas Chromatographic Method <sup>(4)</sup> 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>(4)</sup>
68	Fluorene	1) Liquid-Liquid Extraction, Gas Chromatographic Method <sup>(4)</sup> 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>(4)</sup>
69	Heptachlor	1) Liquid-Liquid Extraction, Gas Chromatographic Method <sup>(4)</sup> 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>(4)</sup>

70 Heptachlor epoxide...

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
70	Heptachlor epoxide	1) Liquid-Liquid Extraction, Gas Chromatographic Method <sup>(4)</sup> 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>(4)</sup>
71	Hexachlorobenzene	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>(4)</sup>
72	Hexachloro-1,3-butadiene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method <sup>(4)</sup>
73	n-Hexane	Purge and Trap Gas Chromatographic/Mass Spectrometric Method <sup>(4)</sup>
74	α-HCH	1) Liquid-Liquid Extraction, Gas Chromatographic Method <sup>(4)</sup> 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>(4)</sup>
75	β-HCH	1) Liquid-Liquid Extraction, Gas Chromatographic Method <sup>(4)</sup> 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>(4)</sup>
76	γ-HCH	1) Liquid-Liquid Extraction, Gas Chromatographic Method <sup>(4)</sup> 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>(4)</sup>
77	Hexachlorocyclopentadiene	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>(4)</sup>
78	Hexachloroethane	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>(4)</sup>
79	Indeno(1,2,3-cd)pyrene	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>(4)</sup>
80	Isophorone	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>(4)</sup>
81	Lead	1) Digestion, Direct Air-Acetylene Flame Method <sup>(4)</sup> 2) Digestion, Electrothermal Atomic Absorption Spectrometric Method <sup>(4)</sup> 3) Digestion, Inductively Coupled Plasma Method <sup>(4)</sup>

82 Manganese...

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
82	Manganese	1) Digestion, Direct Air-Acetylene Flame Method <sup>(4)</sup> 2) Digestion, Electrothermal Atomic Absorption Spectrometric Method <sup>(4)</sup> 3) Digestion, Inductively Coupled Plasma Method <sup>(4)</sup>
83	Mercury	Digestion, Cold-Vapor Atomic Absorption Spectrometric Method <sup>(4)</sup>
84	Methanol	Purge and Trap Gas Chromatographic/Mass Spectrometric Method <sup>(4)</sup>
85	Methoxychlor	Liquid-Liquid Extraction, Gas Chromatographic Method <sup>(4)</sup>
86	Methyl bromide	Purge and Trap Gas Chromatographic/Mass Spectrometric Method <sup>(4)</sup>
87	Methylene chloride	Purge and Trap Gas Chromatographic/Mass Spectrometric Method <sup>(4)</sup>
88	2-Methylphenol	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>(4)</sup>
89	2-Methylnaphthalene	1) Liquid-Liquid Extraction, Gas Chromatographic Method <sup>(4)</sup> 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>(4)</sup>
90	Methyl tert-butyl ether	Purge and Trap Gas Chromatographic/Mass Spectrometric Method <sup>(4)</sup>
91	Naphthalene	1) Liquid-Liquid Extraction, Gas Chromatographic Method <sup>(4)</sup> 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>(4)</sup>
92	Nickel	1) Digestion, Direct Air-Acetylene Flame Method <sup>(4)</sup> 2) Digestion, Electrothermal Atomic Absorption Spectrometric Method <sup>(4)</sup> 3) Digestion, Inductively Coupled Plasma Method <sup>(4)</sup>
93	Nitrobenzene	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>(4)</sup>
94	N-Nitrosodiphenylamine	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>(4)</sup>
95	N-Nitrosodi-n-propylamine	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>(4)</sup>

96 Polychlorinated Biphenyls...

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
96	Polychlorinated Biphenyls - PCB 1016 - PCB 1221 - PCB 1232 - PCB-1242 - PCB-1248 - PCB-1254 - PCB-1260	1) Liquid-Liquid Extraction, Gas Chromatographic Method <sup>(4)</sup> 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>(4)</sup>
97	Pentachlorophenol	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>(4)</sup>
98	pH	Electrometric Method <sup>(4)</sup>
99	Phenanthrene	1) Liquid-Liquid Extraction, Gas Chromatographic Method <sup>(4)</sup> 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>(4)</sup>
100	Phenol	1) Distillation, Chloroform Extraction Method <sup>(4)</sup> 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>(4)</sup>
101	Pyrene	1) Liquid-Liquid Extraction, Gas Chromatographic Method <sup>(4)</sup> 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>(4)</sup>
102	Selenium	1) Digestion, Hydride Generation/Atomic Absorption Spectrometric Method <sup>(4)</sup> 2) Digestion, Inductively Coupled Plasma Method <sup>(4)</sup>
103	Silver	Digestion, Inductively Coupled Plasma Method <sup>(4)</sup>
104	Styrene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method <sup>(4)</sup>
105	1,1,2,2-Tetrachloroethane	Purge and Trap Gas Chromatographic/Mass Spectrometric Method <sup>(4)</sup>
106	Tetrachloroethylene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method <sup>(4)</sup>
107	Toluene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method <sup>(4)</sup>

108 Toxaphene...

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
108	Toxaphene	1) Liquid-Liquid Extraction, Gas Chromatographic Method <sup>(4)</sup> 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>(4)</sup>
109	TPH (C <sub>5</sub> - C <sub>8</sub> )	1) Purge and Trap, Gas Chromatographic Method <sup>(11,21)</sup> 2) Purge and Trap, Gas Chromatographic/Mass spectrometric Method <sup>(11,25)</sup>
110	TPH (C <sub>9</sub> - C <sub>16</sub> )	Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method <sup>(9,21)</sup>
111	TPH (C <sub>16</sub> - C <sub>35</sub> )	Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method <sup>(9,21)</sup>
112	1,2,4-Trichlorobenzene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method <sup>(4)</sup>
113	1,1,1-Trichloroethane	Purge and Trap Gas Chromatographic/Mass Spectrometric Method <sup>(4)</sup>
114	1,1,2-Trichloroethane	Purge and Trap Gas Chromatographic/Mass Spectrometric Method <sup>(4)</sup>
115	Trichloroethylene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method <sup>(4)</sup>
116	2,4,5-Trichlorophenol	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>(4)</sup>
117	2,4,6-Trichlorophenol	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>(4)</sup>
118	1,3,5-Trimethylbenzene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method <sup>(4)</sup>
119	Vanadium	Digestion, Inductively Coupled Plasma Method <sup>(4)</sup>
120	Vinyl acetate	Purge and Trap Gas Chromatographic/Mass Spectrometric Method <sup>(4)</sup>
121	Vinyl chloride	Purge and Trap Gas Chromatographic/Mass Spectrometric Method <sup>(4)</sup>
122	m-Xylene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method <sup>(4)</sup>
123	o-Xylene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method <sup>(4)</sup>

124 p-Xylene...

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
124	p-Xylene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method <sup>(4)</sup>
125	Xylene (Total)	Purge and Trap Gas Chromatographic/Mass Spectrometric Method <sup>(4)</sup>
126	Zinc	1) Digestion, Direct Air-Acetylene Flame Method <sup>(4)</sup> 2) Digestion, Electrothermal Atomic Absorption Spectrometric Method <sup>(4)</sup> 3) Digestion, Inductively Coupled Plasma Method <sup>(4)</sup>

## จากเคมี (ต่อเนื่องจาก) จำนวน 25 รายการ

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
1	Antimony	Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method <sup>(3)</sup>
2	Arsenic	1) Isokinetic Sampling, Digestion, Hydride Generation/Atomic Absorption Spectrometric Method <sup>(4)</sup> 2) Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method <sup>(3)</sup>
3	Cadmium	1) Isokinetic Sampling, Digestion, Direct Air-Acetylene Flame Method <sup>(3)</sup> 2) Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method <sup>(3)</sup>
4	Carbon Monoxide	Instrumental Analyzer Method <sup>(3)</sup>
5	Chlorine	Isokinetic Sampling, Ion Chromatographic Method <sup>(3)</sup>
6	Chromium	1) Isokinetic Sampling, Digestion, Direct Air-Acetylene Flame Method <sup>(3)</sup> 2) Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method <sup>(3)</sup>
7	Cobalt	Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method <sup>(3)</sup>
8	Copper	1) Isokinetic Sampling, Digestion, Direct Air-Acetylene Flame Method <sup>(3)</sup> 2) Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method <sup>(3)</sup>
9	Cresol	Absorption Sampling, Gas Chromatographic Method <sup>(3)</sup>

10 Dioxins/Furans...

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
10	Dioxins/Furans	Isokinetic Sampling <sup>(3)</sup>
11	Hydrogen Chloride	Isokinetic Sampling, Ion Chromatographic Method <sup>(3)</sup>
12	Hydrogen Fluoride	Isokinetic Sampling, Ion Chromatographic Method <sup>(3)</sup>
13	Hydrogen Sulfide	Absorption Sampling, Iodometric Method <sup>(3)</sup>
14	Lead	1) Isokinetic Sampling, Digestion, Direct Air-Acetylene Flame Method <sup>(3)</sup> 2) Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method <sup>(3)</sup>
15	Manganese	1) Isokinetic Sampling, Digestion, Direct Air-Acetylene Flame Method <sup>(3)</sup> 2) Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method <sup>(3)</sup>
16	Mercury	Isokinetic Sampling, Digestion, Cold-Vapor Atomic Absorption Spectrometric Method <sup>(3)</sup>
17	Nickel	1) Isokinetic Sampling, Digestion, Direct Air-Acetylene Flame Method <sup>(3)</sup> 2) Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method <sup>(3)</sup>
18	Opacity	Ringelmann's Method <sup>(1)</sup>
19	Oxides of Nitrogen	1) Absorption Sampling, Phenoldisulfonic acid Method <sup>(3)</sup> 2) Instrumental Analyzer Method <sup>(3)</sup>
20	Selenium	1) Isokinetic Sampling, Digestion, Hydride Generation/Atomic Absorption Spectrometric Method <sup>(3)</sup> 2) Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method <sup>(3)</sup>
21	Sulfur Dioxide	1) Absorption Sampling, Barium-Thorin Titrimetric Method <sup>(5)</sup> 2) Instrumental Analyzer Method <sup>(3)</sup>
22	Sulfuric Acid	Isokinetic Sampling, Barium-Thorin Titrimetric Method <sup>(3)</sup>
23	Total Suspended Particulate	Isokinetic Sampling, Gravimetric Method <sup>(3)</sup>
24	Vanadium	Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method <sup>(3)</sup>
25	Xylene	1) Bag Sampling, Gas Chromatographic Method <sup>(3)</sup> 2) Adsorption Sampling, Gas Chromatographic Method <sup>(3)</sup>

สิ่งปนเปื้อน...

สิ่งปลูกหรือวัสดุที่ไม่ใช้แล้ว จำนวน 35 รายการ

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
1	Aldrin	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method <sup>(2,9,22)</sup> 2) Ultrasonic Extraction, Gas Chromatographic Method <sup>(10,22)</sup>
2	Antimony	Digestion, Inductively Coupled Plasma Method <sup>(7,13)</sup>
3	Arsenic	1) Waste Extraction, Digestion, Hydride Generation/Atomic Absorption Spectrometric Method <sup>(2,6,13)</sup> 2) Waste Extraction, Digestion, Inductively Coupled Plasma Method <sup>(2,6,13)</sup> 3) Digestion, Hydride Generation/Atomic Absorption Spectrometric Method <sup>(7,13)</sup> 4) Digestion, Inductively Coupled Plasma Method <sup>(7,13)</sup>
4	Barium	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method <sup>(2,6,13)</sup> 2) Digestion, Inductively Coupled Plasma Method <sup>(7,13)</sup>
5	Beryllium	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method <sup>(7,13)</sup> 2) Digestion, Inductively Coupled Plasma Method <sup>(7,13)</sup>
6	Cadmium	1) Waste Extraction, Digestion, Flame Atomic Absorption Spectrometric Method <sup>(2,6,14)</sup> 2) Waste Extraction, Digestion, Inductively Coupled Plasma Method <sup>(2,6,13)</sup> 3) Digestion, Flame Atomic Absorption Spectrometric Method <sup>(7,14)</sup> 4) Digestion, Inductively Coupled Plasma Method <sup>(7,13)</sup>
7	Chlordane	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method <sup>(2,9,22)</sup> 2) Ultrasonic Extraction, Gas Chromatographic Method <sup>(10,22)</sup>
8	Chromium	1) Waste Extraction, Digestion, Flame Atomic Absorption Spectrometric Method <sup>(2,6,14)</sup> 2) Waste Extraction, Digestion, Inductively Coupled Plasma Method <sup>(2,6,13)</sup>

3) Digestion,...

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
9	Chromium (III)	3) Digestion, Flame Atomic Absorption Spectrometric Method <sup>(7,14)</sup> 4) Digestion, Inductively Coupled Plasma Method <sup>(7,13)</sup> 1) Waste Extraction, Digestion, Flame Atomic Absorption Spectrometric Method; Waste Extraction, Colorimetric Method; Calculation <sup>(2,6,14,16)</sup> 2) Waste Extraction, Digestion, Inductively Coupled Plasma Method; Waste Extraction, Colorimetric Method; Calculation <sup>(2,6,13,14)</sup> 3) Digestion, Flame Atomic Absorption Spectrometric Method; Alkaline Digestion, Colorimetric Method; Calculation <sup>(7,8,13,14)</sup> 4) Digestion, Inductively Coupled Plasma Method; Alkaline Digestion, Colorimetric Method; Calculation <sup>(7,8,13,14)</sup>
10	Chromium (VI)	1) Waste Extraction, Colorimetric Method <sup>(2,14)</sup> 2) Alkaline Digestion, Colorimetric Method <sup>(8,14)</sup>
11	Cobalt	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method <sup>(2,6,13)</sup> 2) Digestion, Inductively Coupled Plasma Method <sup>(7,13)</sup>
12	Copper	1) Waste Extraction, Digestion, Flame Atomic Absorption Spectrometric Method <sup>(2,6,14)</sup> 2) Waste Extraction, Digestion, Inductively Coupled Plasma Method <sup>(2,6,13)</sup> 3) Digestion, Flame Atomic Absorption Spectrometric Method <sup>(7,14)</sup> 4) Digestion, Inductively Coupled Plasma Method <sup>(7,13)</sup>
13	2,4-D	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method <sup>(2,9,22)</sup> 2) Ultrasonic Extraction, Gas Chromatographic Method <sup>(10,22)</sup>
14	DDD	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method <sup>(2,9,22)</sup> 2) Ultrasonic Extraction, Gas Chromatographic Method <sup>(10,22)</sup>

15 DDE,...

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
15	DDE	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method <sup>(2,9,22)</sup> 2) Ultrasonic Extraction, Gas Chromatographic Method <sup>(10,22)</sup>
16	DDT	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method <sup>(2,9,22)</sup> 2) Ultrasonic Extraction, Gas Chromatographic Method <sup>(10,22)</sup>
17	Dieldrin	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method <sup>(2,9,22)</sup> 2) Ultrasonic Extraction, Gas Chromatographic Method <sup>(10,22)</sup>
18	Endrin	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method <sup>(2,9,22)</sup> 2) Ultrasonic Extraction, Gas Chromatographic Method <sup>(10,22)</sup>
19	Heptachlor	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method <sup>(2,9,22)</sup> 2) Ultrasonic Extraction, Gas Chromatographic Method <sup>(10,22)</sup>
20	Lead	1) Waste Extraction, Digestion, Flame Atomic Absorption Spectrometric Method <sup>(2,6,14)</sup> 2) Waste Extraction, Digestion, Inductively Coupled Plasma Method <sup>(2,6,13)</sup> 3) Digestion, Flame Atomic Absorption Spectrometric Method <sup>(7,14)</sup> 4) Digestion, Inductively Coupled Plasma Method <sup>(7,13)</sup>
21	Lindane	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method <sup>(2,9,22)</sup> 2) Ultrasonic Extraction, Gas Chromatographic Method <sup>(10,22)</sup>
22	Mercury	1) Waste Extraction, Digestion, Cold-Vapor Atomic Absorption Spectrometric Method <sup>(2,17)</sup> 2) Waste Extraction, Digestion, Inductively Coupled Plasma Method <sup>(2,6,13)</sup>

3) Digestion,...

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
23	Methoxychlor	3) Digestion, Cold-Vapor Atomic Absorption Spectrometric Method <sup>(18)</sup> 4) Digestion, Inductively Coupled Plasma Method <sup>(7,13)</sup> 5) Thermal Decomposition Amalgamation and Atomic Absorption Spectrometric Method <sup>(19)</sup>
24	Molybdenum	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method <sup>(2,6,13)</sup> 2) Digestion, Inductively Coupled Plasma Method <sup>(7,13)</sup>
25	Nickel	1) Waste Extraction, Digestion, Flame Atomic Absorption Spectrometric Method <sup>(2,6,14)</sup> 2) Waste Extraction, Digestion, Inductively Coupled Plasma Method <sup>(2,6,13)</sup> 3) Digestion, Flame Atomic Absorption Spectrometric Method <sup>(7,14)</sup> 4) Digestion, Inductively Coupled Plasma Method <sup>(7,13)</sup>
26	Polychlorinated Biphenyls - Aroclor 1016 - Aroclor 1221 - Aroclor 1232 - Aroclor 1242 - Aroclor 1248 - Aroclor 1254 - Aroclor 1260 - 2-Chlorobiphenyl - 2,3-Dichlorobiphenyl - 2,2',5'-Trichlorobiphenyl - 2,4',5'-Trichlorobiphenyl - 2,2',3,5'-Tetrachlorobiphenyl - 2,2',5,5'-Tetrachlorobiphenyl - 2,3',4,4'-Tetrachlorobiphenyl - 2,2',3,4,5'-Pentachlorobiphenyl	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method <sup>(2,9,22)</sup> 2) Ultrasonic Extraction, Gas Chromatographic Method <sup>(10,22)</sup>

- 2,2',4,5,5'-

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
27	- 2,2',4,5,5'-Pentachlorobiphenyl - 2,3,3',4',6'-Pentachlorobiphenyl - 2,2',3,4,4',5'-Hexachlorobiphenyl - 2,2',3,4,5,5'-Hexachlorobiphenyl - 2,2',3,5,5',6'-Hexachlorobiphenyl - 2,2',4,4',5,5'-Hexachlorobiphenyl - 2,2',3,3',4,4',5'-Heptachlorobiphenyl - 2,2',3,4,4',5,5'-Heptachlorobiphenyl - 2,2',3,4,4',5,6'-Heptachlorobiphenyl - 2,2',3,4',5,5',6'-Heptachlorobiphenyl - 2,2',3,3',4,4',5,5',6'-Nonachlorobiphenyl Pentachlorophenol	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>(2,9,28)</sup> 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>(10,26)</sup> Electrometric Method <sup>(31,32)</sup>
28	pH	
29	Selenium	1) Waste Extraction, Digestion, Hydride Generation/Atomic Absorption Spectrometric Method <sup>(2,6,25)</sup> 2) Waste Extraction, Digestion, Inductively Coupled Plasma Method <sup>(2,6,13)</sup> 3) Digestion, Hydride Generation/Atomic Absorption Spectrometric Method <sup>(7,29)</sup> 4) Digestion, Inductively Coupled Plasma Method <sup>(7,13)</sup>

30 Silver...

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
30	Silver	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method <sup>(2,6,13)</sup> 2) Digestion, Inductively Coupled Plasma Method <sup>(7,13)</sup>
31	Thallium	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method <sup>(2,6,13)</sup> 2) Digestion, Inductively Coupled Plasma Method <sup>(7,13)</sup>
32	Toxaphene	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method <sup>(2,9,22)</sup> 2) Ultrasonic Extraction, Gas Chromatographic Method <sup>(10,22)</sup>
33	Trichloroethylene	1) Waste Extraction, Purge and Trap, Gas Chromatographic/Mass Spectrometric Method <sup>(2,12,23)</sup> 2) Purge and Trap, Gas Chromatographic/Mass Spectrometric Method <sup>(12,23)</sup>
34	Vanadium	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method <sup>(2,6,13)</sup> 2) Digestion, Inductively Coupled Plasma Method <sup>(7,13)</sup>
35	Zinc	1) Waste Extraction, Digestion, Flame Atomic Absorption Spectrometric Method <sup>(2,6,14)</sup> 2) Waste Extraction, Digestion, Inductively Coupled Plasma Method <sup>(2,6,13)</sup> 3) Digestion, Flame Atomic Absorption Spectrometric Method <sup>(7,14)</sup> 4) Digestion, Inductively Coupled Plasma Method <sup>(7,13)</sup>

คืน จำนวน 125 รายการ

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
1	Acenaphthene	1) Ultrasonic Extraction, Gas Chromatographic Method <sup>(10,24)</sup> 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>(10,26)</sup>
2	Acetone	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method <sup>(12,23)</sup>

3 Aldrin...

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
3	Aldrin	1) Ultrasonic Extraction, Gas Chromatographic Method <sup>(10,22)</sup> 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>(10,26)</sup>
4	Anthracene	1) Ultrasonic Extraction, Gas Chromatographic Method <sup>(10,26)</sup> 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>(10,26)</sup>
5	Antimony	Digestion, Inductively Coupled Plasma Method <sup>(7,13)</sup>
6	Arsenic	1) Digestion, Hydride Generation/Atomic Absorption Spectrometric Method <sup>(7,15)</sup> 2) Digestion, Inductively Coupled Plasma Method <sup>(7,13)</sup>
7	Atrazine	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>(10,26)</sup>
8	Barium	Digestion, Inductively Coupled Plasma Method <sup>(7,13)</sup>
9	Benz(a)anthracene	1) Ultrasonic Extraction, Gas Chromatographic Method <sup>(10,26)</sup> 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>(10,26)</sup>
10	Benzene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method <sup>(12,23)</sup>
11	Benzo(b)fluoranthene	1) Ultrasonic Extraction, Gas Chromatographic Method <sup>(10,26)</sup> 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>(10,26)</sup>
12	Benzo(k)fluoranthene	1) Ultrasonic Extraction, Gas Chromatographic Method <sup>(10,26)</sup> 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>(10,26)</sup>
13	Benzoic acid	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>(10,26)</sup>
14	Benzo(a)pyrene	1) Ultrasonic Extraction, Gas Chromatographic Method <sup>(10,26)</sup> 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>(10,26)</sup>

15 Benzo(g,h,i)perylene...

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
15	Benzo(g,h,i)perylene	1) Ultrasonic Extraction, Gas Chromatographic Method <sup>(10,22)</sup> 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>(10,26)</sup>
16	Beryllium	Digestion, Inductively Coupled Plasma Method <sup>(7,13)</sup>
17	Bis(2-chloroethyl)ether	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>(10,26)</sup>
18	Bis(2-ethylhexyl)phthalate	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>(10,26)</sup>
19	Bromodichloromethane	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method <sup>(12,23)</sup>
20	Bromoform	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method <sup>(12,23)</sup>
21	Butanol	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method <sup>(12,23)</sup>
22	Butyl benzyl phthalate	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>(10,26)</sup>
23	Cadmium	1) Digestion, Flame Atomic Absorption Spectrometric Method <sup>(7,14)</sup> 2) Digestion, Inductively Coupled Plasma Method <sup>(7,13)</sup>
24	Carbazole	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>(10,26)</sup>
25	Carbon disulfide	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method <sup>(12,23)</sup>
26	Carbon tetrachloride	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method <sup>(12,23)</sup>
27	Chlordane	1) Ultrasonic Extraction, Gas Chromatographic Method <sup>(10,22)</sup> 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>(10,26)</sup>
28	p-Chloroaniline	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>(10,26)</sup>
29	Chlorobenzene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method <sup>(12,23)</sup>
30	Chlorodibromomethane	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method <sup>(12,23)</sup>

31 Chloroform...

ลำดับ	สารพิษ	วิธีวิเคราะห์
31	Chloroform	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method <sup>(12,25)</sup>
32	2-Chlorophenol	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>(10,26)</sup>
33	Chromium	1) Digestion, Flame Atomic Absorption Spectrometric Method <sup>(7,14)</sup> 2) Digestion, Inductively Coupled Plasma Method <sup>(7,13)</sup>
34	Chromium (III)	1) Digestion, Flame Atomic Absorption Spectrometric Method; Alkaline Digestion, Colorimetric Method; Calculation <sup>(7,8,13,14)</sup> 2) Digestion, Inductively Coupled Plasma Method; Alkaline Digestion, Colorimetric Method; Calculation <sup>(7,8,13,14)</sup>
35	Chromium (VI)	Alkaline Digestion, Colorimetric Method <sup>(8,14)</sup>
36	Chrysene	1) Ultrasonic Extraction, Gas Chromatographic Method <sup>(10,26)</sup> 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>(10,26)</sup>
37	Cyanide	Extraction, Distillation, Colorimetric Method <sup>(28,29,30)</sup>
38	2,4-D	Ultrasonic Extraction, Gas Chromatographic Method <sup>(27)</sup>
39	DDD	1) Ultrasonic Extraction, Gas Chromatographic Method <sup>(10,22)</sup> 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>(10,26)</sup>
40	DDE	1) Ultrasonic Extraction, Gas Chromatographic Method <sup>(10,22)</sup> 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>(10,26)</sup>
41	DDT	1) Ultrasonic Extraction, Gas Chromatographic Method <sup>(10,22)</sup> 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>(10,26)</sup>
42	Dibenz(a,h)anthracene	1) Ultrasonic Extraction, Gas Chromatographic Method <sup>(10,26)</sup> 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>(10,26)</sup>

43 Di-n-butyl phthalate...

ลำดับ	สารพิษ	วิธีวิเคราะห์
43	Di-n-butyl phthalate	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>(10,26)</sup>
44	1,2-Dichlorobenzene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method <sup>(12,25)</sup>
45	1,3-Dichlorobenzene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method <sup>(12,25)</sup>
46	1,4-Dichlorobenzene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method <sup>(12,25)</sup>
47	3,3'-Dichlorobenzidine	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>(10,26)</sup>
48	1,1-Dichloroethane	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method <sup>(12,25)</sup>
49	1,2-Dichloroethane	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method <sup>(12,25)</sup>
50	1,1-Dichloroethylene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method <sup>(12,25)</sup>
51	cis-1,2-Dichloroethylene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method <sup>(12,25)</sup>
52	trans-1,2-Dichloroethylene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method <sup>(12,25)</sup>
53	2,4-Dichlorophenol	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>(10,26)</sup>
54	1,2-Dichloropropane	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method <sup>(12,25)</sup>
55	1,3-Dichloropropane	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method <sup>(12,25)</sup>
56	1,3-Dichloropropene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method <sup>(12,25)</sup>
57	Dieldrin	1) Ultrasonic Extraction, Gas Chromatographic Method <sup>(10,22)</sup> 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>(10,26)</sup>
58	Diethyl phthalate	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>(10,26)</sup>
59	2,4-Dimethylphenol	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>(10,26)</sup>

60 2,4-Dinitrophenol...

ลำดับ	สารพิษ	วิธีวิเคราะห์
60	2,4-Dinitrophenol	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>(10,26)</sup>
61	2,4-Dinitrotoluene	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>(10,26)</sup>
62	2,6-Dinitrotoluene	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>(10,26)</sup>
63	Di-n-Octyl phthalate	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>(10,26)</sup>
64	Endosulfan	1) Ultrasonic Extraction, Gas Chromatographic Method <sup>(10,22)</sup> 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>(10,26)</sup>
65	Endrin	1) Ultrasonic Extraction, Gas Chromatographic Method <sup>(10,22)</sup> 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>(10,26)</sup>
66	Ethylbenzene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method <sup>(12,25)</sup>
67	Fluoranthene	1) Ultrasonic Extraction, Gas Chromatographic Method <sup>(10,26)</sup> 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>(10,26)</sup>
68	Fluorene	1) Ultrasonic Extraction, Gas Chromatographic Method <sup>(10,26)</sup> 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>(10,26)</sup>
69	Heptachlor	1) Ultrasonic Extraction, Gas Chromatographic Method <sup>(10,22)</sup> 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>(10,26)</sup>
70	Heptachlor epoxide	1) Ultrasonic Extraction, Gas Chromatographic Method <sup>(10,22)</sup> 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>(10,26)</sup>

71 Hexachlorobenzene...

ลำดับ	สารพิษ	วิธีวิเคราะห์
71	Hexachlorobenzene	1) Ultrasonic Extraction, Gas Chromatographic Method <sup>(10,22)</sup> 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>(10,26)</sup>
72	Hexachloro-1,3-butadiene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method <sup>(12,25)</sup>
73	n-Hexane	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method <sup>(12,25)</sup>
74	α-HCH	1) Ultrasonic Extraction, Gas Chromatographic Method <sup>(10,22)</sup> 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>(10,26)</sup>
75	β-HCH	1) Ultrasonic Extraction, Gas Chromatographic Method <sup>(10,22)</sup> 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>(10,26)</sup>
76	γ-HCH	1) Ultrasonic Extraction, Gas Chromatographic Method <sup>(10,22)</sup> 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>(10,26)</sup>
77	Hexachlorocyclopentadiene	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>(10,26)</sup>
78	Hexachloroethane	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>(10,26)</sup>
79	Indeno(1,2,3-cd)pyrene	1) Ultrasonic Extraction, Gas Chromatographic Method <sup>(10,26)</sup> 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>(10,26)</sup>
80	Isophorone	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>(10,26)</sup>
81	Lead	1) Digestion, Flame Atomic Absorption Spectrometric Method <sup>(7,14)</sup> 2) Digestion, Inductively Coupled Plasma Method <sup>(7,13)</sup>
82	Manganese	1) Digestion, Flame Atomic Absorption Spectrometric Method <sup>(7,14)</sup> 2) Digestion, Inductively Coupled Plasma Method <sup>(7,13)</sup>

83 Mercury...

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
83	Mercury	1) Digestion, Cold-Vapor Atomic Absorption Spectrometric Method <sup>(18)</sup> 2) Digestion, Inductively Coupled Plasma Method <sup>(7,13)</sup> 3) Thermal Decomposition Amalgamation and Atomic Absorption Spectrometric Method <sup>(19)</sup>
84	Methanol	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method <sup>(12,23)</sup>
85	Methoxychlor	1) Ultrasonic Extraction, Gas Chromatographic Method <sup>(10,22)</sup> 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>(10,26)</sup>
86	Methyl bromide	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method <sup>(12,25)</sup>
87	Methylene chloride	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method <sup>(12,25)</sup>
88	2-Methylphenol	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>(10,26)</sup>
89	2-Methylnaphthalene	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>(10,26)</sup>
90	Methyl tert-butyl ether	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method <sup>(12,25)</sup>
91	Naphthalene	1) Ultrasonic Extraction, Gas Chromatographic Method <sup>(10,24)</sup> 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>(10,26)</sup>
92	Nickel	1) Digestion, Flame Atomic Absorption Spectrometric Method <sup>(7,14)</sup> 2) Digestion, Inductively Coupled Plasma Method <sup>(7,13)</sup>
93	Nitrobenzene	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>(10,26)</sup>
94	N-Nitrosodiphenylamine	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>(10,26)</sup>
95	N-Nitrosodi-n-propylamine	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>(10,26)</sup> <i>ตรวจ</i>

96 Polychlorinated Biphenyls...

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
96	Polychlorinated Biphenyls - Aroclor 1016 - Aroclor 1221 - Aroclor 1232 - Aroclor 1242 - Aroclor 1248 - Aroclor 1254 - Aroclor 1260 Polychlorinated Biphenyls - 2-Chlorobiphenyl - 2,3-Dichlorobiphenyl - 2,2',5'-Trichlorobiphenyl - 2,4',5'-Trichlorobiphenyl - 2,2',3,5'-Tetrachlorobiphenyl - 2,2',5,5'-Tetrachlorobiphenyl - 2,3',4,4'-Tetrachlorobiphenyl - 2,2',3,4,5'-Pentachlorobiphenyl - 2,2',4,5,5'-Pentachlorobiphenyl - 2,3,3',4',6'-Pentachlorobiphenyl - 2,2',3,4,4',5'-Hexachlorobiphenyl - 2,2',3,4,5,5'-Hexachlorobiphenyl - 2,2',3,5,5',6'-Hexachlorobiphenyl - 2,2',4,4',5,5'-Hexachlorobiphenyl - 2,2',3,3',4,4',5'-Heptachlorobiphenyl - 2,2',3,4,4',5,5'-Heptachlorobiphenyl - 2,2',3,4,4',5,6'-Heptachlorobiphenyl	1) Ultrasonic Extraction, Gas Chromatographic Method <sup>(10,23)</sup> 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>(10,26)</sup>  Ultrasonic Extraction, Gas Chromatographic Method <sup>(10,23)</sup> <i>ตรวจ</i>

- 2,2',3,4',5,5',6...

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
97	- 2,2',3,4',5,5',6'-Heptachlorobiphenyl - 2,2',3,3',4,4',5,5',6'-Nonachlorobiphenyl Pentachlorophenol	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>(10,26)</sup>
98	Phenanthrene	1) Ultrasonic Extraction, Gas Chromatographic Method <sup>(10,26)</sup> 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>(10,26)</sup>
99	Phenol	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>(10,26)</sup>
100	Pyrene	1) Ultrasonic Extraction, Gas Chromatographic Method <sup>(10,24)</sup> 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>(10,26)</sup>
101	Selenium	1) Digestion, Hydride Generation/Atomic Absorption Spectrometric Method <sup>(7,22)</sup> 2) Digestion, Inductively Coupled Plasma Method <sup>(7,13)</sup>
102	Silver	Digestion, Inductively Coupled Plasma Method <sup>(7,13)</sup>
103	Styrene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method <sup>(12,25)</sup>
104	1,1,2,2-Tetrachloroethane	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method <sup>(12,25)</sup>
105	Tetrachloroethylene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method <sup>(12,25)</sup>
106	Toluene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method <sup>(12,25)</sup>
107	Toxaphene	Ultrasonic Extraction, Gas Chromatographic Method <sup>(10,22)</sup>
108	TPH (C <sub>5</sub> -C <sub>8</sub> )	1) Purge and Trap, Gas Chromatographic Method <sup>(12,21)</sup> 2) Purge and Trap, Gas Chromatographic/Mass Spectrometric Method <sup>(12,25)</sup>
109	TPH (C <sub>9</sub> -C <sub>18</sub> )	Ultrasonic Extraction, Gas Chromatographic Method <sup>(10,21)</sup>
110	TPH (C <sub>19</sub> -C <sub>33</sub> )	Ultrasonic Extraction, Gas Chromatographic Method <sup>(10,21)</sup>
111	1,2,4-Trichlorobenzene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method <sup>(12,25)</sup> <i>ตรวจ</i>

112 1,1,1-Trichloroethane...

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
112	1,1,1-Trichloroethane	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method <sup>(12,25)</sup>
113	1,1,2-Trichloroethane	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method <sup>(12,25)</sup>
114	Trichloroethylene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method <sup>(12,25)</sup>
115	2,4,5-Trichlorophenol	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>(10,26)</sup>
116	2,4,6-Trichlorophenol	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>(10,26)</sup>
117	1,3,5-Trimethylbenzene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method <sup>(12,25)</sup>
118	Vanadium	Digestion, Inductively Coupled Plasma Method <sup>(7,13)</sup>
119	Vinyl acetate	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method <sup>(12,25)</sup>
120	Vinyl chloride	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method <sup>(12,25)</sup>
121	m-Xylene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method <sup>(12,25)</sup>
122	o-Xylene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method <sup>(12,25)</sup>
123	p-Xylene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method <sup>(12,25)</sup>
124	Xylene (Total)	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method <sup>(12,25)</sup>
125	Zinc	1) Digestion, Flame Atomic Absorption Spectrometric Method <sup>(7,14)</sup> 2) Digestion, Inductively Coupled Plasma Method <sup>(7,13)</sup>

## เอกสารอ้างอิง

- กระทรวงอุตสาหกรรม. ประกาศกระทรวงอุตสาหกรรม, พ.ศ. 2549. เรื่อง กำหนดค่าปริมาณเคมีภัณฑ์ที่เจือปนในอากาศที่ระบายออกจากรถยนต์ของหน่วยงานราชการที่ใช้แก๊สเป็นเชื้อเพลิง.
- ราชกิจจานุเบกษา. 4 ธันวาคม 2549. เล่มที่ 123 ตอนพิเศษ 125 ง.
- กระทรวงอุตสาหกรรม. ประกาศกระทรวงอุตสาหกรรม, พ.ศ. 2548. เรื่อง การกำจัดสิ่งปฏิกูลหรือวัสดุที่ไม่ใช้แล้ว.ราชกิจจานุเบกษา. 25 มกราคม 2549. เล่มที่ 123 ตอนพิเศษ 114 ง.

3. สมาคมวิศวกรที่งานสิ่งแวดล้อมแห่งประเทศไทย. คู่มือวิเคราะห์น้ำเสีย. พิมพ์ครั้งที่ 4. กรุงเทพมหานคร: วิศวกรรมเคมี, 2547.
4. APHA, AWWA, WEF. **Standard Methods for the Examination of Water and Wastewater**. 23<sup>rd</sup> ed. Washington, DC: APHA, 2017.
5. United States Environmental Protection Agency. **Standards of Performance for New Stationary Sources**. 40 CFR 60. Appendix A, 2019.
6. United States Environmental Protection Agency. **Test Methods for Evaluation Solid Waste Physical/Chemical Methods**. SW-846, 1997.
7. United States Environmental Protection Agency. **Test Methods for Evaluation Solid Waste Physical/Chemical Methods. Acid Digestion of Sediments, Sludges, and Soils**. SW-846 Method 3050B, 1996.
8. United States Environmental Protection Agency. **Test Methods for Evaluation Solid Waste Physical/Chemical Methods. Alkaline Digestion for Hexavalent Chromium**. SW-846 Method 3060A, 1996.
9. United States Environmental Protection Agency. **Test Methods for Evaluation Solid Waste 3. Physical/Chemical Methods. Separatory Funnel Liquid-Liquid Extraction**. SW-846 Method 3510C, 1996.
10. United States Environmental Protection Agency. **Test Methods for Evaluation Solid Waste Physical/Chemical Methods. Ultrasonic Extraction**. SW-846 Method 3550C, 2007.
11. United States Environmental Protection Agency. **Test Methods for Evaluation Solid Waste Physical/Chemical Methods. Purge and Trap for Aqueous Samples**. SW-846 Method 5030C, 2003.
12. United States Environmental Protection Agency. **Test Methods for Evaluation Solid Waste Physical/Chemical Methods. Closed System Purge and Trap and Extraction for Volatile Organics in Soil and Waste Sample**. SW-846 Method 5035A, 2000.
13. United States Environmental Protection Agency. **Test Methods for Evaluation Solid Waste Physical/Chemical Methods. Inductively Coupled Plasma-Optical Emission Spectrometry**. SW-846 Method 6010D, 2014.
14. United States Environmental Protection Agency. **Test Methods for Evaluation Solid Waste Physical/Chemical Methods. Flame Atomic Absorption Spectrophotometry**. SW-846 Method 7000B, 2007.
15. United States Environmental Protection Agency. **Test Methods for Evaluation Solid Waste Physical/Chemical Methods. Arsenic (Atomic Absorption, Gaseous Hydride)**. SW-846 Method 7061A, 1992.

16, United States...

16. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Chromium, Hexavalent (Colorimetric)**. SW-846 Method 7196A, 1992.
17. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Mercury in Liquid Waste (Manual Cold Vapor Technique)**. SW-846 Method 7470A, 1994.
18. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Mercury in Solid or Semisolid Waste (Manual Cold-Vapor Technique)**. SW-846 Method 7471B, 1998.
19. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Mercury in Solids and Solutions by Thermal Decomposition, Amalgamation, and Atomic Absorption Spectrophotometry**. SW-846 Method 7473, 2007.
20. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Selenium (Atomic Absorption, Borohydride Reduction)**. SW-846 Method 7742, 1994.
21. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Nonhalogenated Organics Using GC/FID**. SW-846 Method 8015D, 2003.
22. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Organochlorine Pesticides by Gas Chromatography**. SW-846 Method 8081B, 2007.
23. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Polychlorinated Biphenyls (PCBs) by Gas Chromatography**. SW-846 Method 8082A, 2007.
24. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Polynuclear Aromatic Hydrocarbons**. SW-846 Method 8100, 1980.
25. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Volatile Organic Compounds by Gas Chromatography/Mass Spectrometry**. SW-846 Method 8260D, 2018.
26. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Semivolatile Organic Compounds by Gas Chromatography/Mass Spectrometry**. SW-846 Method 8270E, 2018.
27. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Chlorinated Herbicides by GC Using Methylation or Pentafluorobenzoylation Derivatization**. SW-846 Method 8151A, 1996. *Small*

28. United States...

28. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Total and Amenable Cyanide : Distillation**. SW-846 Method 9010C, 2004.
29. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Cyanide Extraction Procedure for Solids and Oils**. SW-846 Method 9013A, 2014.
30. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Cyanide in Waters and Extracts using Titrimetric and Manual Spectrophotometric Procedures**. SW-846 Method 9014, 2014.
31. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **pH Electrometric Measurement**. SW-846 Method 9040C, 2004.
32. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Soil and Waste pH**. SW-846 Method 9045D, 2004.



**TG 6**

东方汽轮机有限公司  
DONGFANG TURBINE Co., Ltd.  
中华人民共和国

