

ภาคผนวก จ

---

สรุปเอกสารการสอบเทียบอุปกรณ์เครื่องมือ

**CERTIFICATE OF ANALYSIS**

**EPA PROTOCOL GAS**

**Cylinder No. : EB0145030**

## CERTIFICATE OF ANALYSIS Grade of Product: EPA Protocol

Part Number: E03N199E15AC0U4  
Cylinder Number: EB0145030  
Laboratory: 124 - Plumsteadville - PA  
PGVP Number: A12021  
Gas Code: CH4,PPN,BALN  
Reference Number: 160-40224242-1  
Cylinder Volume: 144.4 CF  
Cylinder Pressure: 2015 PSIG  
Valve Outlet: 350  
Certification Date: Oct 15, 2021  
Expiration Date: Oct 15, 2029

Certification performed in accordance with "EPA Traceability Protocol for Assay and Certification of Gaseous Calibration Standards (May 2012)" document EPA 000/R-12/031, using the assay procedures listed. Analytical Methodology does not require correction for analytical uncertainty. This cylinder has a full analytical uncertainty as stated below with a confidence level of 95%. There are no significant impurities which affect the use of this calibration mixture. All concentrations are on a mole/mole basis unless otherwise noted.

Do Not Use This Cylinder below 100 psig, i.e. 0.7 megapascals.

ANALYTICAL RESULTS					
Component	Requested Concentration	Actual Concentration	Protocol Method	Total Relative Uncertainty	Assay Dates
METHANE	180.0 PPM	177.0 PPM	G1	+/- 1.0% NIST Traceable	10/15/2021
PROPANE	185.0 PPM	187.0 PPM	G1	+/- 1.0% NIST Traceable	10/15/2021
NITROGEN	Balance				
CALIBRATION STANDARDS					
Type	Lot ID	Cylinder No	Concentration	Uncertainty	Expiration Date
NTRM	08011503	K002564	246.7 PPM METHANE/AIR	+/- 0.6%	May 15, 2025
NTRM	200602-06	6162660Y	243.3 PPM PROPANE/AIR	+/- 0.5%	Mar 17, 2027
ANALYTICAL EQUIPMENT					
Instrument/Make/Model	Analytical Principle		Last Multipoint Calibration		
Nicolet IS50 FTIR AUP2110295 CH4	FTIR		Oct 13, 2021		
Nicolet IS50 FTIR AUP2110295 C3H8	FTIR		Oct 14, 2021		

### Triad Data Available Upon Request

NOTES:  
Gross Weight: 28.0 Kg  
Net Weight: 4.9 Kg  
PO# 5221004861



**COPY**

*Michael A. Huber*  
Approved for Release

**DRY GAS METER MC572V**

**Serial No. : 0504003**



## Certificate Of Calibration

Method 5 Pre-Test Console Calibration - Cubic meter (m3)

## Meter Console Information

Console Model : MC572V  
 Console serial : 0504003  
 DGM Model # : SK25EX  
 DGM Serial # : 00009854

## Calibration Condition

Cal Date : 22-Apr-24  
 Due Date : 23-Apr-25  
 Cal Report No. : WDS-SV6704001  
 Ambient Temp (°C) : 25  
 Pressure (mm Hg) : 758  
 Relative Humidity (%) : 60

## Factors/Conversion

Std Temp (°K) : 298  
 Std Pressure (mm Hg) : 760  
 K<sub>1</sub> (K/mm Hg) : 0.3857

## Reference Equipment

WTM Model : W-NKoDa-5B WTM Cal Due Date : Dec. 2023  
 WTM Serial : 600245 Gamma : 1.0000

## UUT Meter (DGM)

## Reference Meter (WTM)

Run Time (minutes)	DGM Orifice (mm H <sub>2</sub> O)	Volume		Outlet Temp		Volume		Outlet Temp	
		Initial	Final	Initial	Final	Initial	Final	Initial	Final
15.00	13.0	144.5926	144.7699	26	27	60.06607	60.24392	29	28
10.00	25.0	144.8168	144.9795	27	27	60.29098	60.45472	27	27
8.00	50.0	145.0164	145.2002	28	28	60.49135	60.67317	29	27
7.00	80.0	145.2238	145.4291	28	28	60.69691	60.90186	29	28
5.00	120.0	145.4909	145.6692	28	29	60.96349	61.14145	27	26

## Standardized Data

## Calibration Results

Test Meter		Reference Meter		Correction Factor		Flow Rate		VH@ (mm H <sub>2</sub> O)
Std Volume	Std Flow Rate	Std Volume	Std Flow Rate	"Gamma"	Variation	Std & Corr	0.0212 SCMM	Variation
V <sub>std</sub> (m <sup>3</sup> )	Q <sub>std</sub> (m <sup>3</sup> /min)	V <sub>ref</sub> (m <sup>3</sup> )	Q <sub>ref</sub> (m <sup>3</sup> /min)	(Y)	(ΔY)	Q <sub>ref</sub> (m <sup>3</sup> /min)	ΔH <sub>sc</sub>	ΔΔH <sub>sc</sub>
0.173	0.012	0.173	0.012	0.997	0.003	0.012	43.309	-0.858
0.159	0.016	0.160	0.016	1.004	0.011	0.016	43.381	-0.787
0.179	0.022	0.176	0.022	0.984	-0.009	0.022	45.447	1.280
0.201	0.029	0.199	0.028	0.989	-0.005	0.028	44.202	0.035
0.175	0.035	0.174	0.035	0.994	0.000	0.035	44.497	0.330

Pass/Fail Result: Pass

Note: For Calibration Factor Y, the ratio of the reading of the calibration meter to the dry gas meter, acceptable tolerance of individual values from the average is ±0.02.

Note: For ΔH<sub>sc</sub>, orifice pressure differential that equals to 0.75cm (0.0212m<sup>3</sup>/min) at standard temperature and pressure, acceptable tolerance of individual values from the average is ±0.2 inches (5.1mm) H<sub>2</sub>O.

Approved By: \_\_\_\_\_

(Patpasu Chaisana)  
 Service Manager

Date: 22-Apr-24

COPY

## Certificate of Calibration - Supplemental

METHOD 5 PRE-TEST CONSOLE CALIBRATION

## Nomenclature

P<sub>0</sub> - Barometric Pressure  
 DGM - Dry Gas Meter  
 K<sub>1</sub> - Constant based on standard temp and press  
 O - Run time, in minutes  
 P<sub>m</sub> - ΔH (Meter Pressure, gauge)  
 V<sub>m</sub> - Volume collected by test meter, corrected for STP  
 Q<sub>m(std)</sub> - Calculated flow rate of test meter  
 K' - Critical orifice coefficient  
 P<sub>w</sub> - Measured pressure of reference meter  
 t<sub>w</sub> - Temperature measured in reference meter  
 t<sub>m</sub> - Temperature measured in test meter  
 Y - Ratio of volume collected from test meter and orifice  
 sc - Scaling Factor  
 Counts<sub>sc</sub> - Number of pulse counts, standardized  
 Counts<sub>total</sub> - Number of raw pulse counts of a calibration run

## Equations

$$V_{w(std)} = Y * K_1 \frac{V_{m(std)} * P_{m} - P_{w}}{T_w}$$

$$V_{m(std)} = Counts_{std} * Y_{sc(avg)}$$

$$Counts_{std} = K_1 \frac{Counts_{total} * (P_{bar} + \frac{P_{m}}{100})}{T_w}$$


$$Q_{w(std)} = \frac{V_{w(std)}}{t}$$

$$K_1 = \frac{T_{std}}{P_{std}}$$

$$Y = \frac{V_{w(std)}}{V_{m(std)}}$$


$$Y_{sc} = \frac{P_{w} - 0.0011696 * P_{m} + \frac{P_{m}}{100}}{T_w} \left( \frac{T_w - t}{T_{std}} \right)$$

## Calibration Train

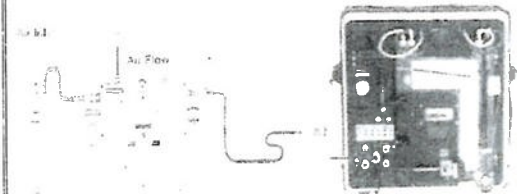

## Calibration Graphs

## Meter Pressure vs Flowrate

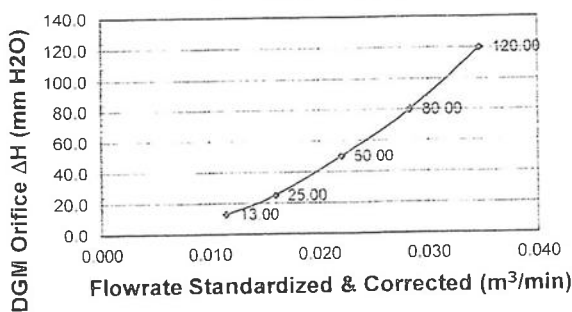


Console Serial

0504003

Console Model

MC572V

## Meter Gamma vs Flowrate

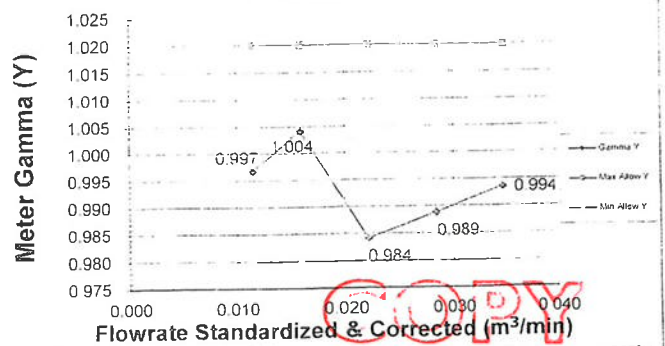

Console Serial

0504003

Console Model

MC572V



WISDOM SCIENCE

TEMPERATURE DISPLAY CALIBRATION

Meter Console Information

Console Model	MC572V
Console serial	0504003
Temp Indicator Model	765-KF
Temp Indicator Serial	JC05630

Calibration Conditions

Cal Date	22-Apr-24
Due Date	23-Apr-25
Cal Report No	WDS-SV8704001
Ambient Temp (°C)	25
Pressure (mm Hg)	758
Humidity (%)	60

Reference Equipment

Temp Meter Model	Fuke 714B
Serial No	60590035
Cal Date	07-Apr-24
Temp Meter Model	Fuke 179
Serial No	58620112
Cal Date	06-Feb-24

Temperature Sensor Calibration

Reference Point	Rel Thermometer Temperature °C	Thermocouple Display Temperature °C	Temperature Difference °C
#			
1	-18.0	-17.0	1.0
2	38.0	37.0	1.0
3	93.0	93.0	0.0
4	149.0	150.0	-1.0
5	260.0	259.0	1.0
6	371.0	372.0	-1.0
7	482.0	482.0	0.0
8	593.0	593.0	0.0
9	816.0	815.0	1.0
10	1038.0	1038.0	0.0
Maximum <sup>1</sup>			1.0

Note

<sup>1</sup> For valid test results, the maximum difference between temperature readings should be  $\leq 1.0^{\circ}\text{C}$  (EPA Method 5, Section 6.1.1.8).  
Perform all TC Channel calibrations. Except meter (DGM) channel

PASS

DGM Out Temperature Sensor Calibration

Temperature point	Rel Thermometer Temperature °C	Thermocouple Display Temperature °C	Temperature Difference °C
#			
Ice	0.0	1.0	-1.0
Ambient	26.5	26.0	0.5
Heat	109.3	110.0	-0.7
Difference Range			
Temp Difference		$\pm 2^{\circ}\text{F}$ or $\pm 1^{\circ}\text{C}$	

PASS

Note

The temperatures of the thermocouple and reference thermometers shall agree to within  $\pm 2^{\circ}\text{F}$  (EPA Method 5, section 10.5)

Approved By :

( Patpasu Chaisana )  
Service Manager

WISDOM SCIENCE

COPY

**DRY GAS METER XC-572-OV**

**Serial No. : A2204323**

## Certificate Of Calibration

Method 5 Pre-Test Console Calibration - Cubic meter (m3)

## Meter Console Information

Console Model : XC-572-OV  
 Console serial : A2204323  
 DGM Model #: SK25EX  
 DGM Serial #: 00008294

## Calibration Condition

Cal. Date: 22-May-24  
 Due Date: 22-May-25  
 Cal. Report No : WDS-SV6704018  
 Ambient Temp (°C): 25  
 Pressure (mm Hg): 758  
 Relative Humidity (%): 60

## Factors/Conversion

Std Temp (°K): 298  
 Std. Pressure (mm Hg): 760  
 K<sub>1</sub> (K/mm Hg): 0.3857

## Reference Equipment

WTM Model: W-NKDa-5B WTM Cal Due Date: Dec. 2024  
 WTM Serial: 600245 Gamma: 1.0000

## UUT Meter (DGM)

Run Time (minutes)	DGM Orifice (mm H <sub>2</sub> O)	Volume		Outlet Temp		Volume		Outlet Temp	
		Initial	Final	Initial	Final	Initial	Final	Initial	Final
15.00	13.0	194.6567	194.8274	26	27	61.39400	61.56423	28	27
10.00	25.0	195.0941	195.2514	28	28	61.82541	61.98088	29	28
8.00	50.0	195.2786	195.4572	28	28	62.00769	62.18342	28	27
7.00	80.0	195.4877	195.6846	28	29	62.21353	62.40748	28	27
5.00	120.0	195.7085	195.8796	29	29	62.43108	62.60020	26	27

## Reference Meter (WTM)

## Standardized Data

Test Meter		Reference Meter		Correction Factor		Flow Rate		ΔH@ (mm H <sub>2</sub> O)	
Std. Volume	Std. Flow Rate	Std. Volume	Std. Flow Rate	"Gamma"	Variation	Std & Corr	0.0212 SCMM	Variation	
V <sub>std</sub> (m <sup>3</sup> )	Q <sub>std</sub> m <sup>3</sup> /min	V <sub>ref</sub> (m <sup>3</sup> )	Q <sub>ref</sub> m <sup>3</sup> /min	(Y)	(ΔY)	Q <sub>ref</sub> (m <sup>3</sup> /min)	ΔH <sub>ref</sub>	ΔΔH <sub>ref</sub>	
0.167	0.011	0.166	0.011	0.994	0.008	0.011	47.022	-1.348	
0.153	0.015	0.151	0.015	0.986	0.000	0.015	48.311	-0.059	
0.174	0.022	0.171	0.021	0.981	-0.005	0.021	48.458	0.089	
0.192	0.027	0.189	0.027	0.981	-0.004	0.027	48.869	0.499	
0.167	0.033	0.165	0.033	0.986	0.000	0.033	49.189	0.819	
				0.985	= Y Avg			48.370	ΔH@ Avg

Pass/Fail Result: **Pass**

Note: For Calibration Factor Y the ratio of the reading of the calibration meter to the dry gas meter, acceptable tolerance of individual values from the average is ±0.02

Note: For ΔH<sub>ref</sub>, orifice pressure differential that equates to 0.75cfm (0.0212m<sup>3</sup>/min) at standard temperature and pressure, acceptable tolerance of individual values from the average is ±0.2 inches (5.1mm) H<sub>2</sub>O

Approved By: \_\_\_\_\_

(Palpasu Chaisana)  
 Service Manager

WISDOM SCIENCE

บริษัท วิสโดม ซาเลนซ์ จำกัด แอนด์ เซอร์วิส กรุ๊ป จำกัด  
 WISDOM SCIENCE SALE AND SERVICE GROUP COMPANY LIMITED

Date: 22-May-24

COPY

## Certificate of Calibration - Supplemental

METHOD 5 PRE-TEST CONSOLE CALIBRATION

## Nomenclature

P<sub>b</sub> - Barometric Pressure  
 DGM - Dry Gas Meter  
 K<sub>1</sub> - Constant based on standard temp and press  
 t - Run time, in minutes  
 P<sub>m</sub> - ΔH (Meter Pressure, gauge)  
 V<sub>m</sub> - Volume collected by test meter, corrected for STP  
 Q<sub>mstd</sub> - Calculated flow rate of test meter  
 K' - Critical orifice coefficient  
 P<sub>w</sub> - Measured pressure of reference meter  
 t<sub>w</sub> - Temperature measured in reference meter  
 t<sub>m</sub> - Temperature measured in test meter  
 Y - Ratio of volume collected from test meter and orifice  
 sc - Scaling Factor  
 Counts<sub>std</sub> - Number of pulse counts, standardized  
 Counts<sub>raw</sub> - Number of raw pulse counts of a calibration run

## Equations

$$V_{m(std)} = Y * K_1 \frac{V_w * (P_{bm} + \frac{P_{m(std)}}{1.6})}{T_w}$$

$$V_{m(std)} = Counts_{std} * Y_{avg}$$


$$Counts_{std} = K_1 \frac{Counts_{raw} * (P_{bm} + \frac{P_{m(std)}}{1.6})}{T_m}$$

$$Q_{m(std)} = \frac{V_{m(std)}}{t} \quad Y = \frac{V_{m(std)}}{Counts_{std}}$$

$$K_1 = \frac{T_{std}}{P_{std}} \quad Y = \frac{V_{m(std)}}{Counts_{std}}$$


$$Y = \frac{P_{std} * (1.6 + \frac{P_{m(std)}}{P_{std}})}{P_{m(std)} * (1.6 + \frac{P_{m(std)}}{P_{std}})} * \left( \frac{P_{std}}{P_{m(std)}} \right)$$

## Calibration Train

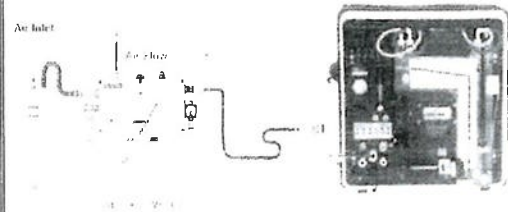

## Calibration Graphs


## Meter Pressure vs Flowrate

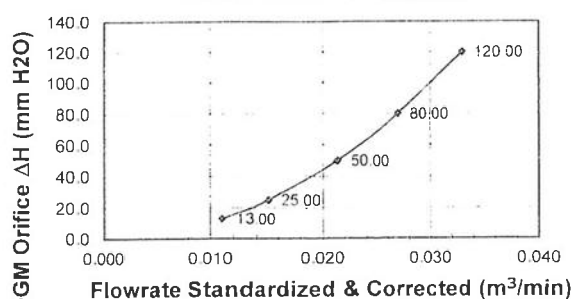

Console Serial: A2204323

Console Model: XC-572-

## Meter Gamma vs Flowrate

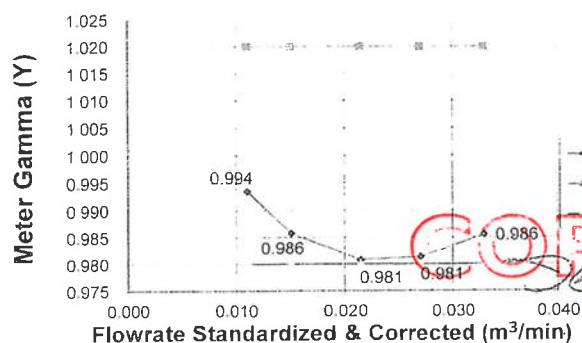

Console Serial: A2204323

Console Model: XC-572-OV



## TEMPERATURE DISPLAY CALIBRATION

## Meter Console Information

Console Model	XC-372-OV
Console serial	A2204323
Temp Indicator Model	765-KF
Temp Indicator Serial	JC35630

## Calibration Conditions

Cal Date	22-May-24
Due Date	22-May-25
Cal Report No	WDS-SVG704018
Ambient Temp (°C)	25
Pressure (mm Hg)	756
Humidity (%)	60

## Reference Equipment

Temp Meter Model	Fuke 7148
Serial No	80590035
Cal Date	07-Apr-24
Temp Meter Model	Fuke 175
Serial No	58620112
Cal Date	06-Feb-24

## Temperature Sensor Calibration

Reference Point	Ref Thermometer Temperature °C	Thermocouple Display Temperature °C	Temperature Difference °C
#			
1	-18.0	-17.0	1.0
2	38.0	37.0	1.0
3	93.0	93.0	0.0
4	149.0	150.0	-1.0
5	260.0	259.0	1.0
6	371.0	372.0	-1.0
7	482.0	482.0	0.0
8	593.0	593.0	0.0
9	816.0	815.0	1.0
10	1038.0	1038.0	0.0
Maximum			1.0

## Note

\* For valid test results, the maximum difference between temperature readings should  $\leq 1.0^{\circ}\text{C}$  ( EPA Method 5, Section 6.1.1.8 )  
Perform all TC Channel calibrations Except meter (DGM) channel

PASS

## DGM Out Temperature Sensor Calibration

Temperature point	Ref Thermometer Temperature °C	Thermocouple Display Temperature °C	Temperature Difference °C
#			
Ice	0.0	1.0	-1.0
Ambient	27.5	27.0	0.5
Heat	108.6	109.0	-0.4
Difference Range			
Temp. Difference	$\pm 2^{\circ}\text{F}$ or $\pm 1^{\circ}\text{C}$		

PASS

## Note

The temperatures of the thermocouple and reference thermometers shall agree to within  $\pm 2^{\circ}\text{F}$  ( EPA Method 5, section 10.5 )

Approved By :

*Palpasu Chaisana*  
( Palpasu Chaisana )  
Service Manager

**WISDOM  
SCIENCE**

บริษัท วิสโดม ไซนซ์ เซลล์ แอนด์ เซอร์วิส จำกัด  
WISDOM SCIENCE SALE AND SERVICE GROUP COMPANY LIMITED

COPY

**DRY GAS METER MC-572-V**

**Serial No. : 1007055**

## Certificate Of Calibration

Method 5 Pre-Test Console Calibration - Cubic meter (m3)

## Meter Console Information

Console Model : MC-572-V  
 Console serial : 1007055  
 DGM Model #: SK25EX  
 DGM Serial #: 0009799

## Calibration Condition

Cal. Date: 04-Aug-24  
 Due Date: 04-Aug-25  
 Cal. Report No.: WDS-SV6707001  
 Ambient Temp (°C): 25  
 Pressure (mm Hg): 758  
 Relative Humidity (%): 60

## Factors/Conversion

Std. Temp. (°K): 298  
 Std. Pressure (mm Hg): 760  
 K<sub>1</sub> (K/mm Hg): 0.3857

## Reference Equipment

WTM Model: W-NKoDa-5B WTM Cal. Due Date: Dec. 2024  
 WTM Serial: 600245 Gamma: 1.0000

## UUT Meter (DGM)

## Reference Meter (WTM)

Run Time (minutes)	DGM Orifice (mm H <sub>2</sub> O)	Volume		Outlet Temp		Volume		Outlet Temp	
		Initial	Final	Initial	Final	Initial	Final	Initial	Final
15.00	13.0	107.7550	107.9221	29	30	68.41024	68.57350	28	27
10.00	25.0	107.9308	108.0876	30	30	68.58202	68.73488	27	27
8.00	50.0	108.1027	108.2822	30	30	68.74958	68.92516	27	27
7.00	80.0	108.3029	108.5061	30	30	68.94550	69.14488	27	27
5.00	120.0	108.5139	108.6908	30	30	69.15251	69.32550	27	27

## Standardized Data

## Calibration Results

Test Meter		Reference Meter		Correction Factor		Flow Rate	ΔH@ (mm H <sub>2</sub> O)	
Std. Volume	Std. Flow Rate	Std. Volume	Std. Flow Rate	"Gamma"	Variation	Std & Corr	0.0212 SCMM	Variation
V <sub>std</sub> (m <sup>3</sup> )	Q <sub>std</sub> m <sup>3</sup> /min	V <sub>ref</sub> (m <sup>3</sup> )	Q <sub>ref</sub> m <sup>3</sup> /min	(Y)	(ΔY)	Q <sub>corrected</sub>	ΔH <sub>sp</sub>	ΔΔH <sub>sp</sub>
0.162	0.011	0.159	0.011	0.982	0.000	0.011	50.751	2.535
0.152	0.015	0.149	0.015	0.982	0.001	0.015	49.300	1.084
0.174	0.022	0.171	0.021	0.983	0.002	0.021	48.061	-0.155
0.197	0.028	0.194	0.028	0.983	0.002	0.028	45.922	-2.293
0.173	0.035	0.169	0.034	0.976	-0.005	0.034	47.046	-1.170

Pass/Fail Result: **Pass**

Note: For Calibration Factor Y, the ratio of the reading of the calibration meter to the dry gas meter, acceptable tolerance of individual values from the average is ±0.02

Note: For ΔH<sub>sp</sub>, orifice pressure differential that equates to 0.75cfm (0.0212m<sup>3</sup>/min) at standard temperature and pressure, acceptable tolerance of individual values from the average is ±0.2 inches (5.1mm) H<sub>2</sub>O

Approved By:

(Patpasu Chaisana)  
 Service Manager

**WISDOM  
SCIENCE**

บริษัท วิสโดม ไซน์แอนด์ เซอร์วิส กรุ๊ป จำกัด  
 WISDOM SCIENCE SALE AND SERVICE GROUP COMPANY LIMITED

Date: 04-Aug-24

COPY

## Certificate of Calibration - Supplemental

METHOD 5 PRE-TEST CONSOLE CALIBRATION

## Nomenclature

## Equations

## Calibration Train

P<sub>a</sub> - Barometric Pressure  
 DGM - Dry Gas Meter  
 K<sub>1</sub> - Constant based on standard temp and press  
 t - Run time, in minutes  
 P<sub>m</sub> - ΔH (Meter Pressure, gauge)  
 V<sub>m</sub> - Volume collected by test meter, corrected for STP  
 Q<sub>m(std)</sub> - Calculated flow rate of test meter  
 K' - Critical orifice coefficient  
 P<sub>w</sub> - Measured pressure of reference meter  
 t<sub>w</sub> - Temperature measured in reference meter  
 t<sub>m</sub> - Temperature measured in test meter  
 Y - Ratio of volume collected from test meter and orifice  
 sc - Scaling Factor  
 Counts<sub>std</sub> - Number of pulse counts, standardized  
 C<sub>total</sub> - Number of raw pulse counts of a calibration run

$$V_{w(std)} = Y * K_1 \frac{V_w * (P_{bar} + \frac{P_w}{1.133})}{T_w}$$

$$V_{m(std)} = Counts_{std} * Y_{scaling}$$


$$Counts_{std} = K_1 \frac{Counts * (P_{bar} + \frac{P_w}{1.133})}{T_m}$$

$$Q_{std} = \frac{V_{w(std)}}{t}$$

$$Y = \frac{V_{m(std)}}{Counts_{std}}$$


$$K_1 = \frac{T_{std}}{P_{std}}$$

$$Metric \Delta H = \frac{P_m}{1.133} * \left( \frac{1}{P_w} - \frac{1}{P_{std}} \right)$$

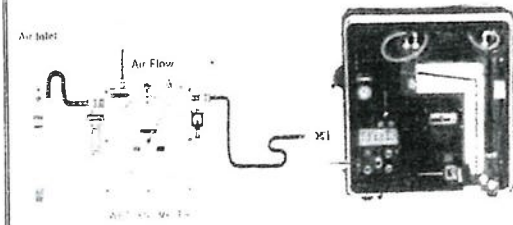

## Calibration Graphs


## Meter Pressure vs Flowrate

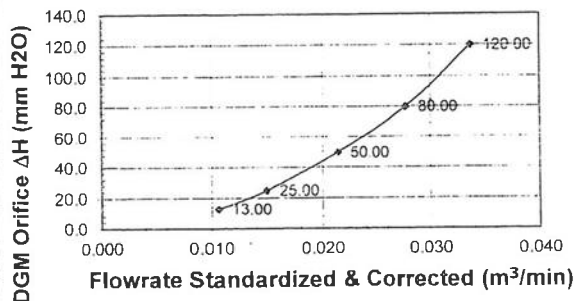

Console Serial: 1007055

Console Model: MC-

## Meter Gamma vs Flowrate

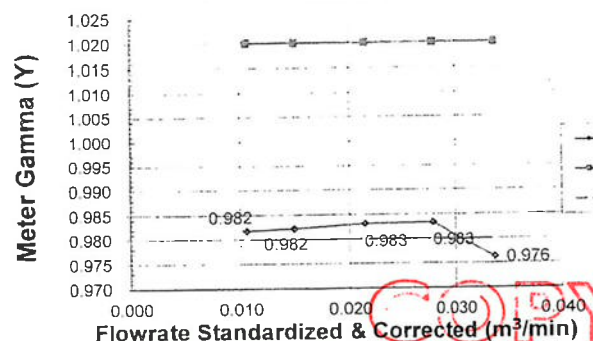

Console Serial: 1007055

Console Model: MC-572-V

**Meter Console Information**

Console Model	MC-572-V
Console serial	1007055
Temp Indicator Model	765-KF
Temp Indicator Serial	JC17852

**Calibration Conditions**

Cal Date	04-Aug-24
Due Date	04-Aug-25
Cal Report No	WDS-SV8707001
Ambient Temp (°C)	25
Pressure (mm Hg)	758
Humidity (%)	60

**Reference Equipment**

Temp Meter Model	Fluke 714B
Serial No	80590035
Cal Date	07-Apr-24
Temp Meter Model	Fluke 179
Serial No	58620112
Cal Date	06-Feb-24

**Temperature Sensor Calibration**

Reference Point	Ref Thermometer Temperature	Thermocouple Display Temperature	Temperature Difference
#	°C	°C	°C
1	-18.0	-18.0	0.0
2	38.0	38.0	0.0
3	93.0	94.0	-1.0
4	149.0	149.0	0.0
5	260.0	261.0	-1.0
6	371.0	372.0	-1.0
7	482.0	482.0	0.0
8	593.0	593.0	0.0
9	816.0	816.0	0.0
10	1038.0	1038.0	0.0
Maximum <sup>1</sup>			1.0

**Note**

<sup>1</sup> For valid test results, the maximum difference between temperature readings should  $\leq 1.0^{\circ}\text{C}$  ( EPA Method 5, Section 6.1.1.8 ).  
Perform all TC Channel calibrations. Except meter (DGM) channel

PASS

**DGM Out Temperature Sensor Calibration**

Temperature point	Ref Thermometer Temperature	Thermocouple Display Temperature	Temperature Difference
#	°C	°C	°C
Ice	0.0	0.0	0.0
Ambient	26.9	27.0	-0.1
Heat	114.5	115.0	-0.5

**Difference Range**

Temp. Difference  $\pm 2^{\circ}\text{F}$  or  $\pm 1^{\circ}\text{C}$

PASS

**Note**

The temperatures of the thermocouple and reference thermometers shall agree to within  $\pm 2^{\circ}\text{F}$  ( EPA Method 5, section 10.5 )

Approved By :

*Parth*  
( Palpasu Chaisana )  
Service Manager

**WISDOM  
SCIENCE**

บริษัท วิสโดม ไซนซ์ เซลล์ แอนด์ เซอร์วิส จำกัด  
WISDOM SCIENCE SALE AND SERVICE GROUP COMPANY LIMITED

**COPY**



**Flue gas Analyzer**

**Testo 350XL**

**Serial No. 01794619/002**



# Calibration Certificate

ENTECH  
Difference For Greater Value

Certificate No.: G 670415  
Date of issue : 25-Jun-24

Instrument description : Flue Gas Analyzer  
Instrument model : Testo 350XL  
Control unit serial no. : 01794619/002  
Instrument serial no. : 01807527/002  
ID no. or control no. : -  
Manufacturer : Testo SE & Co. KGaA  
Probe description : -  
Probe model : -  
Probe serial no. : -  
Customer name : Eastern Thai Consulting 1992 Company Limited  
Customer address : 683 Moo 11, Sukhapibarn 8 Road, Nongkham, Si Racha, Chon Buri 20280

Total pages of certificate : 2 Pages  
Receiving no. : L-242269  
Receiving date. : 19-Jun-24  
Parameter of calibration : Gas Calibration(Oxygen 2.50,10.04,21.02 %vol, Carbon Monoxide 80.18,302,1001 ppm, Nitrogen Dioxide 30.34,81.32, 201.9 ppm, Nitric Oxide 30.01, 151.5, 322.5 ppm, Sulphur Dioxide 50.36, 100.8, 600.8 ppm)

Condition of UUC. : Used  
Ambient condition : All of the Measurement were carried out the stabilized laboratory

Temperature : 23 ±5 °C  
Humidity : 55 ± 15 %RH

Calibration place : 17/121 Soi Ngamwongwan 47 Yaek 48, Toongsonghong, Laksi, Bangkok 10210

Calibration procedure no. : This instrument was calibrated by comparison with Standard gas mixture according to calibration Work Instruction no. WI-CL-28-C

*The calibration certificate expanded uncertainty of measurement is stated as the standard uncertainty of measurement Multiplied by coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%. This certificate is applied only to item under test Environmental condition.*

*This Calibration Certificate may not be reproduced other than in full except with the permission of the issuing laboratory. Calibration certificates without signature and seal not valid and The results relate only to the items tested/calibrated.*

*This calibration certificate documents are traceability to national standards, which realize measurement according to the International System of Units (SI).*

Date of calibration : 24-Jun-24

*Kornchai K.*

Mr. Kwanchai Khandoung  
Calibration Technician

*กนกพร นงนุช*

Mrs. Nongnuch Hamfaifa  
Technical Manager



# Calibration Certificate

Certificate No.: G 670415

Standard References (Table 1)

Standard	Certificate No.	Vendor	Due date
Oxygen ( O2 ) 2.50 % Vol	2412/23	Linde	27-Aug-27
Oxygen ( O2 ) 10.04 % Vol	CG-0153-21	Nimt	18-Nov-26
Oxygen ( O2 ) 21.02 % Vol	CG-0041-22	Nimt	10-Feb-27
Carbon monoxide ( CO ) 80.18 ppm	CG-0002-24	Nimt	11-Jan-29
Carbon monoxide ( CO ) 302 ppm	1915/23	Linde	16-Jun-25
Carbon monoxide ( CO ) 1001 ppm	CG-0085-24	Nimt	22-May-29
Nitrogen Dioxide ( NO2 ) 30.34 ppm	2703/22	Linde	22-Aug-24
Nitrogen Dioxide ( NO2 ) 81.32 ppm	3546/23	Linde	14-Jan-26
Nitrogen Dioxide ( NO2 ) 201.9 ppm	1975/23	Linde	17-Jul-25
Nitric Oxide ( NO ) 30.01 ppm	CG-0014-23	Nimt	19-Feb-25
Nitric Oxide ( NO ) 151.5 ppm	0161/23	Linde	22-Jan-25
Nitric Oxide ( NO ) 322.5 ppm	1974/23	Linde	17-Jul-25
Sulphur Dioxide ( SO2 ) 50.36 ppm	2004/23	Linde	17-Jul-25
Sulphur Dioxide ( SO2 ) 100.8 ppm	3507/22	Linde	09-Nov-24
Sulphur Dioxide ( SO2 ) 600.8 ppm	2003/23	Linde	17-Jul-25

## Measured room conditions

Temperature : 24.1 °C Humidity : 62.8 %RH Pressure : 1005.9 mbar  
Calibration conditions  
Gas Temperature : 24 °C Flow rate : 1,000 ml/min Gas pressure : 1014.7 mbar

Calibration Results (Without adjustment) (Table 2)

Parameter of Standard	Standard Values	Mean of UUC	Error	Uncertainty (±)
O2 (%Vol)	2.50	2.48	-0.02	0.15
O2 (%Vol)	10.04	9.93	-0.11	0.20
O2 (%Vol)	21.02	21.11	0.09	0.30
CO (ppm)	80.18	81	0.82	3.0
CO (ppm)	302	302	0	6.0
CO (ppm)	1001	1002	1	12
NO2 (ppm)	30.34	31.5	1.16	8.0
NO2 (ppm)	81.32	82.3	0.98	8.0
NO2 (ppm)	201.9	201.2	-0.7	12
NO (ppm)	30.01	32	1.99	8.0
NO (ppm)	151.5	155	3.5	8.0
NO (ppm)	322.5	327	4.5	12
SO2 (ppm)	50.36	49	-1.36	6.0
SO2 (ppm)	100.8	100	-0.8	6.0
SO2 (ppm)	600.8	602	1.2	13

Remark : 1 cmol/mol = 1 %vol, 1 µmol/mol = 1 ppm.

## End of Report



**UV/VIS SPECTROPHOTOMETER**

**Model : UV-1800**

**Serial No. : A11635101643 CD**



**Bara Scientific**  
968 U Chu Liang Building Floor 7 Rama4 Road  
Silom Bangkok Bangkok Thailand 10500  
Tel : 02-6324300 Fax : 02-6375496-7  
www.barascientific.com



## Certificate of Calibration

Number of Page(s) 1 of 3

Certificate No. BSCC-UV-146/24  
Equipment UV/Vis Spectrophotometer  
Model UV-1800  
Manufacturer Shimadzu  
Serial No. A11635101643 CD  
ID No. LABE 03/2  
Date of receipt 22 April 2024  
Date of calibration 22 April 2024  
Date of issue 29 April 2024  
Customer name Eastern Thai Consulting 1992 Co., Ltd.  
Address 683 Moo 11, Sukkaphibarn 8 Rd., Nongkham, Sriracha, Chonburi 20230

Temperature (22.9-24.1) °C (On site)  
Humidity (41.7-46.9) %RH (On site)

Equipment condition Good Operation

Calibration Location Analysis Department

Calibration Procedure In-house method WI-UV-702-01 based on ASTM E275-01

Traceability  
Wavelength Accuracy is traceable to certificate No. 116614 and 116613  
Photometric Accuracy is traceable to certificate No. 116210 and 116224  
Stray Light is traceable to certificate No. 116616  
The above certificate are traceable to SI unit through Siam Scientific Ltd.  
(UKAS accredited calibration laboratory NO. 0659)

Calibrated by Mr. Poomjai Korsawatvorakul

Approved by

Mr. Sonthi Temboonsakdi  
Service Manager

The above results are valid exclusively for the calibrated item(s) as mention in this report / certificate  
Advertising the report / Certificate and publicity of the results are prohibited and also shall not be reproduced  
except in full, without written approval of the Bara Scientific Co., Ltd.



**Bara Scientific Co., Ltd.**  
968 U Chu Liang Building Floor 7 Rama4 Road  
Silom Bangkok Bangkok Thailand 10500  
Tel : 02-6324300 Fax : 02-6375496-7  
www.barascientific.com



## Certificate of Calibration

Certificate No. BSCC-UV-146/24

Number of Page(s) 2 of 3

Calibration Results:

### 1. Wavelength Accuracy

Certified Wavelength (nm)	UUC (nm)	Error (nm)	Uncertainty (±nm)
287.71	287.75	0.04	0.18
445.82	445.89	0.07	0.18
536.52	536.50	-0.02	0.18
741.02	741.01	-0.01	0.18
879.41	879.33	-0.08	0.18

### 2. Photometric Accuracy (UV)

Wavelength (nm)	Certified Absorbance (A)	UUC (A)	Error (A)	Uncertainty (±A)
235	0.0000	0.0000	0.0000	0.0075
	0.7415	0.7387	-0.0028	0.0075
257	CNR	CNR	CNR	CNR
	CNR	CNR	CNR	CNR
313	CNR	CNR	CNR	CNR
	CNR	CNR	CNR	CNR
350	0.0000	0.0000	0.0000	0.0075
	0.6406	0.6395	-0.0011	0.0075

\*CNR = Customer not request

The above results are valid exclusively for the calibrated item(s) as mention in this report / certificate  
Advertising the report / Certificate and publicity of the results are prohibited and also shall not be reproduced  
except in full, without written approval of the Bara Scientific Co., Ltd.



**Bara Scientific Co., Ltd.**  
968 U Chu Liang Building Floor 7 Rama4 Road  
Silom Bangkok Bangkok Thailand 10500  
Tel : 02-6324300 Fax : 02-6375496-7  
www.barascientific.com



# Certificate of Calibration

Certificate No. BSCC-UV-146/24 Number of Page(s) 3 of 3

Calibration Results:

## 3. Photometric Accuracy (Visible)

Wavelength (nm)	Certified Absorbance (A)	UUC (A)	Error (A)	Uncertainty (±A)
420.0	0.0000	0.0000	0.0000	0.0042
	0.5715	0.5729	0.0014	0.0042
	0.7087	0.7087	0.0000	0.0042
440.0	1.0987	1.1005	0.0018	0.0042
	0.0000	0.0000	0.0000	0.0042
	0.5561	0.5578	0.0017	0.0042
465.0	0.6968	0.6969	0.0001	0.0042
	1.0757	1.0774	0.0017	0.0042
	CNR	CNR	CNR	CNR
546.1	CNR	CNR	CNR	CNR
	CNR	CNR	CNR	CNR
	CNR	CNR	CNR	CNR
590.0	0.0000	0.0000	0.0000	0.0042
	0.5193	0.5213	0.0020	0.0042
	0.6937	0.6940	0.0003	0.0042
635.0	1.0411	1.0428	0.0017	0.0042
	CNR	CNR	CNR	CNR
	CNR	CNR	CNR	CNR
635.0	0.0000	0.0000	0.0000	0.0042
	0.5605	0.5624	0.0019	0.0042
	0.7579	0.7583	0.0004	0.0042
CNR - Customer not request	1.1131	1.1138	0.0007	0.0042

## 4. Stray Light\*

Standard cut-off wavelength (nm)	Unit Under Calibration(UUC)	
	Wavelength (nm)	Absorbance (A)
201.33±0.11nm	200.80	2.0111

The Stray light transmission reference is less than 1.0%T and Stray light absorbance reference is greater than 2.00A

The measurement uncertainty is base on a standard uncertainty multiplied by a coverage factor k=2 providing a level of confidence of approximately 95%.

\*\*\*End of Certificate\*\*\*

The above results are valid exclusively for the calibrated item(s) as mention in this report / certificate. Advertising the report / Certificate and publicity of the results are prohibited and also shall not be reproduced except in full, without written approval of the Bara Scientific Co., Ltd

COPY

**CERTIFICATE OF ANALYSIS**

**EPA PROTOCOL GAS**

**Cylinder No. : EB0062815**

## CERTIFICATE OF ANALYSIS

### Grade of Product: EPA Protocol

Part Number: E04N199E15ACX9C Reference Number: 82-401135335-1  
Cylinder Number: EB0082815 Cylinder Volume: 144.4 CF  
Laboratory: 124 - Riverton (SAP) - NJ Cylinder Pressure: 2015 PSIG  
PGVP Number: B52018 Valve Outlet: 660  
Gas Code: CO,NO,NOX,SO2,BALN Certification Date: Mar 13, 2018  
Expiration Date: Mar 13, 2026

Certification performed in accordance with "EPA Traceability Protocol for Assay and Certification of Gaseous Calibration Standards (May 2012)" document EPA 600/R-12/531, using the assay procedures listed. Analytical Methodology does not require correction for analytical interference. This cylinder has a total analytical uncertainty as stated below with a confidence level of 95%. There are no significant impurities which affect the use of this calibration mixture. All concentrations are on a volume/volume basis unless otherwise noted.

Do Not Use This Cylinder below 100 psig, i.e. 0.7 megapascals.

ANALYTICAL RESULTS				
Component	Requested Concentration	Actual Concentration	Protocol Method	Total Relative Uncertainty
NOX	50.00 PPM	50.55 PPM	G1	+/- 1.4% NIST Traceable
NITRIC OXIDE	50.00 PPM	50.50 PPM	G1	+/- 1.4% NIST Traceable
SULFUR DIOXIDE	50.00 PPM	51.01 PPM	G1	+/- 1.0% NIST Traceable
CARBON MONOXIDE	2000 PPM	1977 PPM	G1	+/- 1.0% NIST Traceable
NITROGEN	Balance			

CALIBRATION STANDARDS		
Type	Lot ID	Cylinder No
NTRM	16050607	CC442564
PRM	12367	APEX1098237
GMIS	0315201604	CC503358
NTRM	16011025	CC473218
NTRM	12060735	CC356192
The SRM, PRM or RGM noted above is only in reference to the GMS used in the assay and not part of the analysis.		

ANALYTICAL EQUIPMENT		
Instrument/Make/Model	Analytical Principle	Last Multipoint Calibration
Nicolet 6700 APW1100391 CO	FTIR	Feb 08, 2018
Nicolet 6700 APW1100391 NO	FTIR	Feb 15, 2018
Nicolet 6700 APW1100391 NO2	FTIR	Feb 16, 2018
Nicolet 6700 APW1100391 SO2	FTIR	Mar 01, 2018

#### Triad Data Available Upon Request

NOTES:NET WEIGHT: 10.43lbs

GROSS WEIGHT: 60.93lbs

PO# 5218000763

This calibration std. has been certified in accordance with the May 2012 EPA Traceability Protocol, Document EPA-600/R-12/531. All testing processes and measurements conform to the requirements of ISO/IEC 17025 and to Airgas ISO 9001:2000 and relate only to items identified on this certificate. All concentrations are certified to be NIST Traceable with total uncertainty as detailed under Analytical Uncertainty. This document shall not be reproduced in full without written approval of the issuer.



TESTING CERT No. 3082.05

*Don Moran*  
Approved for Release

**SOUND LEVEL CALIBRATOR**

**MODEL : NC-75**

**SERIAL No. : 34302326**



Cert. No. : ACC24014  
Pages : 1 of 3

## Calibration Certificate

Equipment : SOUND CALIBRATOR  
Manufacturer : RION  
Model : NC-75  
Serial No.: 34302326  
ID No.: -

Condition As Found : GOOD

Customer : EASTERN THAI CONSULTING 1992 CO., LTD.  
SAHA GROUP INDUSTRIAL PARK, 683 MOO 11,  
NONGKHAM, SIRACHA, CHONBURI 20230 THAILAND.

Location :  
Ambient Temperature : ( 23.0 ± 3 ) °C  
Pressure : ( 101.3 ± 3 ) kPa  
Relative Humidity : ( 50.0 ± 20 ) %

Received Date : 29 APRIL 2024  
Calibration Date : 16 MAY 2024  
Date of Issue : 20 MAY 2024

Calibrated by : Nathakorn Pisutpaisan

Approved by :   
( Thanakul Petchurai )

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.



Cert. No. : ACC24014  
Job No. : VC67ACW083  
Pages : 2 of 3

Calibration Procedure : CP-AC-03

### Calibration Method :

This equipment was calibrated by follow on IEC-60942-2003 Standard.  
The sound pressure level, frequency and total distortion of the sound calibrator was measured using the reference microphone.



### Condition of this result of calibration :

1. Reference Standard Instruments :

Instrument	Model	Serial No.	Cert. No.	Due Date
Waveform Generator	33511B	MY52302742	EF-0007-24	05-FEB-25
Digital Multimeter	33461A	MY33220104	EEL-BP 21/0267	13-FEB-25
Digital Multimeter	33461A	MY33220076	EEL-BP 20/0267	15-FEB-25
Digital Multimeter	33461A	MY60024273	EEL-BP 22/0267	15-FEB-25
Programmable Attenuator	MAT-1070	62100114	EF-0008-24	05-FEB-25
Condenser Microphone	4180	2977900	AA-1001-24	12-FEB-25
Measuring Amplifier	NA-42KAI	34560495	AA-3001-24	05-FEB-25
Audio Analyzer	AVR-3360A	V744B6069	EF-0009-24	09-FEB-25

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.  
3. This certificate is traceable to the international system of unit maintained at :

- 3.1 National Institute of Metrology (Thailand).
- 3.2 Thailand Institute of Scientific and Technological Research (TISTR).

Cert. No. : ACC24014  
Job No. : VC67AC0083  
Pages : 3 of 3

Result of calibration :

1. Sound pressure level

Specified sound pressure level (dB)	Measured value (dB)	Deviated value (dB)	Uncertainty (dB)	Acceptance limit (dB)
94	94.01	0.01	0.28	0.40

2. Frequency

Specified Frequency (Hz)	Measured value (Hz)	Deviated value (%)	Uncertainty (%)	Acceptance limit (%)
1000	1000.0	0.0	0.1	1.0

3. Total distortion

Measured value (%)	Uncertainty (%)	Acceptance limit (%)
0.31	0.10	3.0

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor  $k = 2$  or any value following calculation, providing a level of confidence of approximately 95 %

End of Calibration Certificate


COPY

Y. Keteh

**SOUND LEVEL METER**

**MODEL : NL-42A**

**SERIAL No. : 00322744**

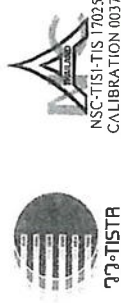

THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-67/0252

MTC No. EEL. BP. 11/0267

## CALIBRATION CERTIFICATE

Submitted by : Eastern Thai Consulting 1992 Co., Ltd.

Address : 683 Moo 11, Sukhapibam 8 Rd., Nongkham, Sriracha, Chonburi, 20230

Calibrated at : Electrical and Electronic Standards Laboratory, Industrial Metrology and Testing Service Centre.

Soi 1C, Bangpoo Industrial Estate, Sukhumvit Rd., A.Muang, Samutprakan 10280.

Instrument Calibrated :

Ambient Environment

Description : Sound Level Meter

Temperature : (23 ± 3) °C

Manufacturer : Rion

Relative Humidity : (50 ± 15) %

Model : NL-42A

Ambient Pressure : (101.325±1.5) kPa

Serial No. : 00322744

Microphone : UC-52 No.196467

Preamplifier : NH-24 No.15476

Standards used :

1. Band Pass Filter Wavetek 752A S/N 90010494.
2. Condenser Microphone Brüel&Kjær 4180 S/N 2889871
3. Decade Attenuator Ando AL-205 S/N 00464602.
4. Function/Arbitrary Waveform Generator Agilent 33220A S/N MY44042668.
5. Digital Function Synthesizer NF Electronic Instruments DF-193A S/N 122037.
6. Digital Multimeter Fluke 8520A S/N 4985007.
7. Pistonphone Rion NC-72 S/N 00402446.
8. Measuring Amplifier Brüel&Kjær 2636 S/N 1537484.

Date of Receipt : 5 Feb. 2024

Date of Calibration : 5 Mar. 2024

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

The results relate only to the items tested/calibrated or value assigned



2 / 9

The results relate only to the items tested/calibrated or value assigned

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.



Date of Calibration : 5 Mar. 2024

The results relate only to the items tested/calibrated or value assigned

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

Head Office  
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,  
Changwat Pathumthani 12120, Thailand  
Tel. (66) 0 2577 9000  
Fax. (66) 0 2577 9009  
E-mail : nrmal@tistr.or.th

Office/Laboratory  
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,  
Amphoe Muang, Changwat Samutprakan 10280, Thailand  
Tel. (66) 0 2323 1672-80 ext. 115, 116  
Fax. (66) 0 2323 9165  
E-mail : mtr@tistr.or.th

Office  
196 Phahonyothin Road, Chulachak, Bangkok 10900,  
Thailand  
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217  
Fax. (66) 0 2579 8592  
E-mail : sumalee@tistr.or.th

FM.BLMTC.002 Rev.1

THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-67/0252

MTC No. EEL. BP. 11/0267

9. Power Amplifier Brüel&Kjær 2706 S/N 1517650.

10. Speaker Tannoy Limited, Great Britain British Patent No. 215300.

11. Digital Multimeter Agilent 34401A S/N MY44005560.

12. Programmable Attenuator Tamagawa TPA-303A S/N 2212.

Calibration Procedure :

This instrument was calibrated by using calibration procedures no CP-102-02 and CP-102-03, which were based on IEC 61672-3 Electroacoustics - Sound Level Meters - Part 3 : Periodic tests (2013). These calibration procedures were related to the electrical and acoustic signal tests. The electrical signal test was carried out with the direct measurement method. The acoustic signal test was performed in an anechoic room with the comparison measurement method.

This instrument has been calibrated against standards maintained at the Electrical and Electronic Standards Laboratory (EEL), which are traceable to the International System of Units through the National Institute of Metrology (Thailand).

The information on actual reading is attached herewith and the uncertainty limits quoted refer to the measured values only.

The reported expanded uncertainty is based upon a standard uncertainty multiplied by a coverage factor k=2, providing a level of confidence of approximately 95%.

1. Absolute Sensitivity

Reference Acoustic Signal (dB)	Measured value (dB)		Deviation value(dB)	Acceptance limit class 2(±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
	Before adjust	After adjust				
113.92	113.8	113.9	0.0	1.0	0.30	N/A

Note: The external calibration adjustment was firstly performed. The internal calibration adjustment was then completed at the display of 114.2 dB.

2. Self-generated noise

2.1 Normal test

Measured value (dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
16.9	0.10	N/A

2.2 The microphone of the sound level meter was replaced by electrical signal input device

Frequency	Measured value (dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Weighting			
A-Weight	12.4	0.10	N/A
C-Weight	17.9	0.10	N/A
Flat	23.1	0.10	N/A

Date of Calibration : 5 Mar. 2024

COPY 3 / 9

The results relate only to the items tested/calibrated or value assigned. Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

3. Acoustical signal test of frequency weightings

Frequency (Hz)	Deviation from frequency response curve(dB)			Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
	A-weight	C-weight	Flat			
125	0.1	0.3	0.4	1.5	0.45	0.6
1 000	0.0	0.0	-0.1	1.0	0.45	0.6
8 000	-0.2	-0.2	-0.2	5.0	0.45	0.7

4. Electrical signal test of frequency weightings

Frequency (Hz)	Deviation from frequency response curve(dB)			Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
	A-weight	C-weight	Flat			
63	0.0	0.1	0.0	2.0	0.20	0.6
125	0.0	0.1	0.0	1.5	0.20	0.6
250	0.0	0.1	0.0	1.5	0.20	0.6
500	0.0	0.1	0.0	1.5	0.20	0.6
1 000	0.0	0.0	0.0	1.0	0.20	0.6
2 000	-0.1	-0.1	-0.2	2.0	0.20	0.6
4 000	-0.3	-0.2	-0.3	3.0	0.20	0.6
8 000	0.0	0.0	-0.1	5.0	0.20	0.7

Date of Calibration : 5 Mar. 2024

COPY 4 / 9

The results relate only to the items tested/calibrated or value assigned. Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.



Request No. 21-67/0252

MTC No. EEL. BP. 11/0267

## 5. Long-term stability

Time	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Begin	94.0	0.0	0.3	0.10	0.1
End	94.0				

## 6. Frequency and time weightings at 1 kHz

## 6.1 Frequency weightings at 1 kHz

Frequency Weighting	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
A-weight	94.0	0.0	0.2	0.20	0.2
C-weight	94.0	0.0	0.2	0.20	0.2
Flat	94.0	0.0	0.2	0.20	0.2

## 6.2 Time weightings at 1 kHz

Frequency Weighting	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Fast	94.0	0.0	0.1	0.20	0.2
Slow	94.0	0.0	0.1	0.20	0.2
Leq	94.0	0.0	0.1	0.20	0.2

Date of Calibration : 5 Mar. 2024

The results relate only to the items tested/calibrated or value assigned  
Advising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR

Request No. 21-67/0252

MTC No. EEL. BP. 11/0267

## 7. Level linearity on the reference level range

Anticipated value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
137	137.1	0.1	1.1	0.30	0.3
136	136.1	0.1	1.1	0.30	0.3
135	135.1	0.1	1.1	0.30	0.3
134	134.1	0.1	1.1	0.30	0.3
129	129.1	0.1	1.1	0.30	0.3
124	124.0	0.0	1.1	0.30	0.3
119	119.1	0.1	1.1	0.30	0.3
114	114.0	0.0	1.1	0.30	0.3
109	109.0	0.0	1.1	0.30	0.3
104	104.1	0.1	1.1	0.30	0.3
99	99.0	0.0	1.1	0.30	0.3
94	94.0	0.0	1.1	0.30	0.3
89	89.0	0.0	1.1	0.30	0.3
84	84.0	0.0	1.1	0.30	0.3
79	79.1	0.1	1.1	0.30	0.3
74	74.1	0.1	1.1	0.30	0.3
69	69.0	0.0	1.1	0.30	0.3
64	64.0	0.0	1.1	0.30	0.3

Date of Calibration : 5 Mar. 2024

The results relate only to the items tested/calibrated or value assigned  
Advising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR

7. Level linearity on the reference level range (cont.)

Anticipated value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
59	59.0	0.0	1.1	0.30	0.3
54	54.0	0.0	1.1	0.30	0.3
49	49.0	0.0	1.1	0.30	0.3
44	44.0	0.0	1.1	0.30	0.3
39	39.0	0.0	1.1	0.30	0.3
34	34.0	0.0	1.1	0.30	0.3
29	29.0	0.0	1.1	0.30	0.3
28	28.0	0.0	1.1	0.30	0.3
27	27.0	0.0	1.1	0.30	0.3
26	26.0	0.0	1.1	0.30	0.3
25	25.0	0.0	1.1	0.30	0.3

8. Level linearity including the level range control

At reference sound level on the reference level range

Range	Anticipated value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
30-130	94.0	94.0	0.0	1.1	0.30	0.3

Date of Calibration : 5 Mar. 2024

COPY 719

The results relate only to the items tested/calibrated or value assigned  
Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

8. Level linearity including the level range control

At reference level at 5 dB greater than the under-range on a level range

Range	Anticipated value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
30-130	35	35.0	0.0	1.1	0.30	0.3

9. Tone burst response

Time Weighting	Toneburst Duration, Tb(ms)	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Fast	200	126.0	0.0	+1.0	0.20	0.3
	2	108.9	-0.1	+1.0; -2.5	0.20	0.3
	0.25	99.9	-0.1	+1.5; -5.0	0.20	0.3
Slow	200	119.5	-0.1	+1.0	0.20	0.3
	2	99.9	-0.1	+1.0; -5.0	0.20	0.3
	200	120.0	0.0	+1.0	0.20	0.3
SEL	2	100.0	0.0	+1.0; -2.5	0.20	0.3
	0.25	90.9	-0.1	+1.5; -5.0	0.20	0.3

Date of Calibration : 5 Mar. 2024

COPY 719

The results relate only to the items tested/calibrated or value assigned  
Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

10. Peak C sound level

Number of cycles in test signal	Anticipated value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2(±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Complete cycle	125.4	125.2	-0.2	3.0	0.20	0.35
Positive half cycle	124.4	124.1	-0.3	2.0	0.20	0.35
Negative half cycle	124.4	124.1	-0.3	2.0	0.20	0.35

11. Overload indication

Measured value (dB)		Deviated value (dB)	Acceptance limit class 2(±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Positive one-half cycle	Negative one-half cycle	value (dB)	limit class 2(±dB)	(±dB)	of measurement (±dB)
136.5	136.5				
		0.0	1.5	0.20	0.25

12. High-level stability

Time	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Begin	129.0	0.0	0.3	0.10	0.1
End	129.0				

Calibrated by : *Witawat Supanich*

(Mr. Witawat Supanich)

Approved by :



Electrical and Electronic Standards Laboratory

Industrial Metrology and Testing Service Centre

Date of Calibration : 5 Mar. 2024

Date of Issue : 6 Mar. 2024

Ref : 2011267020500503003

End of Certificate

9 / 9

The results relate only to the items tested/calibrated or value assigned.  
Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FMBL/MTC.002 Rev.



**SOUND LEVEL METER**

**MODEL : NL-42A**

**SERIAL No. : 00222593**



Cert. No. : ACL24133  
Pages : 1 of 8

## Calibration Certificate

Equipment : SOUND LEVEL METER  
Manufacturer : RION  
Model : NF-42A / Microphone UC-52 / Preamplifier NH-24  
Serial No. : 00222593 / 195905 / 15425  
ID No. :


Condition As Found : GOOD

Customer : EASTERN THAI CONSULTING 1992 CO., LTD.  
SAHA GROUP INDUSTRIAL PARK, 683 MOO 11,  
NONGKHAM, SIRACHA, CHONBURI 20230 THAILAND.

Location :  
Ambient Temperature : ( 23.0 ± 3 ) °C  
Pressure : ( 101.3 ± 3 ) kPa  
Relative Humidity : ( 50.0 ± 20 ) %

Received Date : 29 APRIL 2024  
Calibration Date : 13-17 MAY 2024  
Date of Issue : 20 MAY 2024

Calibrated by : Nathakorn Pisutpaisan

Approved by :   
( Thanakul Petchurai )

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

COPY

Cert. No. : ACL24133  
Job No. : VC67AC0083  
Pages : 2 of 8

Calibration Procedure : CP-AC-01

### Calibration Method :

This equipment was calibrated by follow on IEC-61672-3 (2013) Standard for sound level meter (SLM).  
The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.

For tests results of each items were made by observation of each Instruments display and also with SLM's display.

### Condition of this result of calibration :

1. Reference Standard Instruments :

Instrument	Model	Serial No.	Cert. No.	Due Date
Waveform Generator	33210A	MY48017076	EF-0009-4	05-FEB-25
Waveform Generator	33511B	MY52302742	EF-0007-24	05-FEB-25
Digital Multimeter	33461A	MY53220104	EEL_BP 21/0267	13-FEB-25
Digital Multimeter	33461A	MY53220076	EEL_BP 20/0267	15-FEB-25
Digital Multimeter	34461A	MY60024273	EEL_BP 22/0267	15-FEB-25
Programmable Attenuator	MA-T-1070	62100114	EF-0008-24	05-FEB-25
Condenser Microphone	4180	2977900	AA-1001-24	12-FEB-25
Measuring Amplifier	NA-42KAJ	34560495	AA-3001-24	05-FEB-25

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.  
3. This certificate is traceable to the international system of unit maintained at :

- 3.1 National Institute of Metrology (Thailand).
- 3.2 Thailand Institute of Scientific and Technological Research (TISTR).

COPY



Cert. No. : ACL24133  
Job No. : VC67AC0083  
Pages : 3 of 8

Summary of Measurement Result :

Parameter	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	0.2	N/A
2. Self-generated noise	0.2	N/A
3. Acoustical signal tests of frequency weightings		
125 Hz	0.3	0.6
1000 Hz	0.3	0.6
8000 Hz	0.3	0.7
4. Electrical signal tests of frequency weightings		
For 10 Hz to 4 kHz	0.3	0.6
For > 4 kHz to 10 kHz	0.3	0.7
For > 10 kHz to 20 kHz	-	1.0
5. Frequency and time weightings at 1 kHz	0.2	0.2
6. Long - term stability	0.1	0.1
7. Level linearity on the reference level range	0.2	0.3
8. Level linearity including the level range control	0.2	0.3
9. Tone burst response	0.2	0.3
10. Peak C sound level	0.2	0.35
11. Overload indication	0.2	0.25
12. High level stability	0.1	0.1

COPY

Y. Petcha.

Cert. No. : ACL24133  
Job No. : VC67AC0083  
Pages : 4 of 8

Result of calibration :

**1. Absolute sensitivity**

Reference Acoustic Signal ( dB )	Measured Value ( dB )	Deviation ( dB )	Acceptance Limit ( dB )
93.9 (93.98)	93.9	0.0	±0.3

**2. Self-generated noise**

2.1 Normal test

Measured Value ( dB )
14.2

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Measured value ( dB )
A - weight	12.0
C - weight	18.5
Flat	24.0

**3. Acoustical signal tests of frequency weightings**

Meter free-field acoustic response at a level of 84 dB

Frequency ( Hz )	Deviation from various frequency weighting response curve (dB)		
	Flat	C-weight	A-weight
125	0.0	0.1	0.1
1000	-0.1	-0.1	-0.1
8000	0.5	0.6	0.6
Acceptance Limits			±1.5
			±1.0
			±5.0

COPY

Y. Petcha.

## 4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency ( Hz )	Deviation from various frequency weighting response curve (dB)		
	Flat	C-weight	A-weight
63	-0.1	0.0	-0.1
125	0.0	0.1	0.0
250	0.0	0.0	0.0
500	0.0	0.1	0.0
1000	0.0	0.0	0.0
2000	0.0	0.1	0.0
4000	0.0	0.0	0.0
8000	0.0	0.1	0.1

## 5. Frequency and time weightings at 1 kHz

5.1 Frequency weightings at 1 kHz

Frequency Weighting	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	94.0	94.0	0.0	$\pm 0.2$
C - weight	94.0	94.0	0.0	$\pm 0.2$
Flat	94.0	94.0	0.0	$\pm 0.2$

5.2 Time weighting at 1 kHz

Frequency Weighting	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Fast	94.0	94.0	0.0	$\pm 0.1$
Slow	94.0	94.0	0.0	$\pm 0.1$
Leq	94.0	94.0	0.0	$\pm 0.1$

## 6. Long - term stability

Frequency Weighting	SLM Display at initial ( dB )	SLM Display at final ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	94.0	94.0	0.0	$\pm 0.3$

## 7. Level linearity on the reference level range

Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
137.0	137.0	0.0	$\pm 1.1$
136.0	136.0	0.0	$\pm 1.1$
135.0	135.0	0.0	$\pm 1.1$
134.0	134.0	0.0	$\pm 1.1$
133.0	133.0	0.0	$\pm 1.1$
132.0	132.0	0.0	$\pm 1.1$
131.0	131.0	0.0	$\pm 1.1$
129.0	129.0	0.0	$\pm 1.1$
124.0	124.0	0.0	$\pm 1.1$
119.0	119.0	0.0	$\pm 1.1$
114.0	114.0	0.0	$\pm 1.1$
109.0	109.0	0.0	$\pm 1.1$
104.0	104.0	0.0	$\pm 1.1$
99.0	99.0	0.0	$\pm 1.1$
94.0	94.0	0.0	$\pm 1.1$
89.0	89.0	0.0	$\pm 1.1$
84.0	84.0	0.0	$\pm 1.1$
79.0	79.0	0.0	$\pm 1.1$
74.0	74.0	0.0	$\pm 1.1$
69.0	69.0	0.0	$\pm 1.1$
64.0	64.0	0.0	$\pm 1.1$
59.0	59.0	0.0	$\pm 1.1$
54.0	54.0	0.0	$\pm 1.1$
49.0	49.0	0.0	$\pm 1.1$
44.0	44.0	0.0	$\pm 1.1$
39.0	39.0	0.0	$\pm 1.1$
34.0	34.0	0.0	$\pm 1.1$
30.0	29.9	-0.1	$\pm 1.1$
29.0	28.9	-0.1	$\pm 1.1$
28.0	27.9	-0.1	$\pm 1.1$
27.0	26.9	-0.1	$\pm 1.1$
26.0	25.9	-0.1	$\pm 1.1$
25.0	24.9	-0.1	$\pm 1.1$

COPY

P. Petcha



## 8. Level linearity including the level range control

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Auto	94.0	94.0	0.0	±1.1

## 9. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Cycle	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.1	0.1	±1.0
Slow	2	8	108.0	108.0	0.0	1.5 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
SEL	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.0	0.0	±1.0

## 10. Peak C sound level

Number of cycle in test signal	Anticipated Value (dB)	Measured Value, L <sub>peak</sub> (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	±3.0
One	136.4	135.8	-0.6	±3.0

Number of cycle in test signal	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	±2.0
Positive half cycle	135.4	135.2	-0.2	±2.0
Negative half cycle	135.4	135.2	-0.2	±2.0

## 11. Overload indication

Measured value ( dB )		Deviated Value ( dB )	Acceptance Limits ( dB )
Positive one-half cycle	Negative one-half cycle	89.7	0.1
89.6			±1.5

## 12. High level stability

Frequency Weighting	SLM Display at initial ( dB )	SLM Display at final ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor  $k = 2$   
or any value following calculation, providing a level of confidence of approximately 95 %

End of Calibration Certificate

COPY

COPY

7. Petcha.

7. Petcha.

**ANALYTICAL BALANCE (DU)**

**Model : XS205DU**

**Serial No. : 1126323724**



Certificate No. : 23-148799  
Sample Code : 23-56200-001

## CERTIFICATE OF CALIBRATION

Customer : EASTERN THAI CONSULTING 1992 CO., LTD.  
683 Moo 11, Sukhapibarn 8 Rd., Nongkham,  
Sriracha, Chonburi 20230

Location of Calibration : EASTERN THAI CONSULTING 1992 CO., LTD.  
(Analytical Balance Room)

Equipment : ELECTRONIC BALANCE

Manufacturer : METTLER TOLEDO

Model : XS205DU

Serial No. : 1126323724

ID No. : LABE 05/1

Date of Receipt : 22 December 2023

Date of Calibration : 22 December 2023

Calibrated by Mr. Somwang Sangdee  
Scientist

Approved by (Mr. Somchai Neampunt)  
Signed for Director

Issue date 25 December 2023

The uncertainties are for a confidence probability of approximately 95%.

The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Asia Medical and Agricultural Laboratory and Research Center Public Company Limited (AMARC).



Certificate No. : 23-148799  
Sample Code : 23-56200-001

## REPORT OF CALIBRATION

Equipment : ELECTRONIC BALANCE  
Manufacturer : METTLER TOLEDO  
Model : XS205DU  
Capacity : Max 81 g / 220 g  
Resolution : 0.01 mg / 0.1 mg  
Serial No. : 1126323724  
ID No. : LABE 05/1

## Result of Calibration

## 1. Test weight and repeatability of reading

Repeatability is a measure of the ability of a balance to supply the same result in repetitive weighings with one and the same load under the same measurement condition. The measurement of the repeatability must include both the balance specifications and the ambient (vibration, fluctuating air current/temperature/humidity, etc.) Operator handling of the balance is also included in the standard deviation.

Unit : g	Range : 80	<input checked="" type="checkbox"/> Before adjustment	<input checked="" type="checkbox"/> After adjustment
<input type="checkbox"/> No adjustment	Nominal value	40	80
<input checked="" type="checkbox"/> Adjustment	Standard weight	40.000054	80.000048
	Average reading of indicator	40.00026	80.00037
	Standard deviation	0.000015	0.000016

Unit : g	Range : 200	<input checked="" type="checkbox"/> Before adjustment	<input checked="" type="checkbox"/> After adjustment
<input type="checkbox"/> No adjustment	Nominal value	100	200
<input checked="" type="checkbox"/> Adjustment	Standard weight	100.000042	200.000041
	Average reading of indicator	100.0003	200.0004
	Standard deviation	0.00005	0.00005

COPY

Certificate No. : 23-148799  
Sample Code : 23-56200-001

Page 3 of 4

## REPORT OF CALIBRATION

## Result of Calibration

## 2. Sensitivity or value of a scale division

Change in the output variable of a measuring instrument divided by the associated change in the input variable.

Unit : g

Range : 80

Range : 200

Test Point	Sensitivity, S	Test Point	Sensitivity, S
0	1.00748	0	1.0274
40	0.98753	100	0.9975
80	0.99751	200	0.9975

## 3. Departure of indication from nominal value, Linearity

Unit : g

Nominal Value	Standard Value	Average Reading of Indicator	Correction Value	Expanded Uncertainty	Coverage Factor (k)
Unload	0.0000000	0.00000	0.00000	0.000012	2.05
0.01	0.0100025	0.01000	0.00000	0.000012	2.05
0.1	0.1000019	0.10001	-0.00001	0.000013	2.03
1	1.0000125	1.00001	0.00000	0.000015	2.02
5	5.0000208	5.00004	-0.00002	0.000021	2.00
10	10.000004	10.00008	-0.00008	0.000026	2.00
20	20.000030	20.00011	-0.00008	0.000036	2.00
50	50.000014	50.00014	-0.00013	0.000068	2.00
100	100.000042	100.0001	-0.0001	0.00016	2.00
150	150.000056	150.0001	0.0000	0.00022	2.00
200	200.000041	200.0002	-0.0002	0.00027	2.00

The result expanded uncertainty of measurement  $U$  is stated as the standard uncertainty of measurement multiplied by the coverage factor  $k$ , which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty of measurement has been determined in accordance with UKAS M3003.

Certificate No. : 23-148799  
Sample Code : 23-56200-001

Page 4 of 4


## REPORT OF CALIBRATION

## Result of Calibration :

## 4. Eccentric or off-centre loading

Deviation of the measurement value through off - center (eccentric) loading. The corner load increases with the weight of the load and its removal from the center of the pan support.

Weighing pan	<input type="radio"/> Circle	Test weight : 50 and 100
	<input type="radio"/> Triangular	
	<input checked="" type="radio"/> Rectangular	
Range	80	200
Position	Reading of indicator	Reading of indicator
1	50.00015	100.0001
2	50.00022	100.0001
3	50.00008	100.0001
4	50.00002	100.0000
5	50.00016	100.0002
6	50.00014	100.0001
Maximum difference	0.00013	0.0001

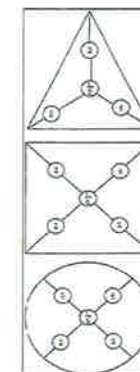

## Condition of Calibration

1. Calibration Method : WI-DL-004 base on UKAS LAB 14: 2019

2. This result of calibration was found accurate as shown on date and place of calibration only.

3. Condition of Calibration tem: Normal

4. This certification is traceable to the International System of Unit maintained at :

Through the reference standard laboratory of Asia Medical and Agricultural Laboratory and Research Center Public Company Limited (Instrument number 1).

## 5. Reference standard instrument :

Instrument	Class	ID No.	Certificate No.	Due Date
1) STANDARD WEIGHT 1 mg to 1 kg	E2	LB-WE-79	23-105642	10 September 2024

End of Report

6. Ambient conditions	Min	Max
Temperature (°C)	22.8	23.0
Relative Humidity (%Rh)	43.5	51.1
Air pressure (hPa)	1012.5	1014.5



**ANALYTICAL BALANCE**

**Model : SECURA224-1S**

**Serial No. : 0036707137**



Certificate No. : 23-148800  
Sample Code : 23-56200-002

## CERTIFICATE OF CALIBRATION

Customer : EASTERN THAI CONSULTING 1992 CO., LTD.  
683 Moo 11, Sukhapibarn 8 Rd., Nongkham,  
Sriracha, Chonburi 20230

Location of Calibration : EASTERN THAI CONSULTING 1992 CO., LTD.  
(Analytical Balance Room)

Equipment : ELECTRONIC BALANCE

Manufacturer : SARTORIUS

Model : SECURA224-1S

Serial No. : 0036707137

ID No. : LABE 05/2

Date of Receipt : 22 December 2023

Date of Calibration : 22 December 2023

Calibrated by Mr. Somwang Sangdee  
Scientist

Approved by (Mr. Somchai Neampunt)  
Signed for Director

Issue date : 25 December 2023

The uncertainties are for a confidence probability of approximately 95%.

The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Asia Medical and Agricultural Laboratory and Research Center Public Company Limited (AMARC).



Certificate No. : 23-148800  
Sample Code : 23-56200-002

## REPORT OF CALIBRATION

Equipment : ELECTRONIC BALANCE  
Manufacturer : SARTORIUS  
Model : SECURA224-1S  
Capacity : Max 220 g  
Resolution : 0.0001 g  
Serial No. : 0036707137  
ID No. : LABE 05/2

## Result of Calibration

## 1. Test weight and repeatability of reading

Repeatability is a measure of the ability of a balance to supply the same result in repetitive weighings with one and the same load under the same measurement condition. The measurement of the repeatability must include both the balance specifications and the ambient (vibration, fluctuating air current/temperature/humidity, etc.) Operator handling of the balance is also included in the standard deviation.

Unit : g	Range : 220	<input checked="" type="checkbox"/> Before adjustment	<input checked="" type="checkbox"/> After adjustment
	Nominal value	100	200
<input type="checkbox"/> No adjustment	Standard weight	100.000042	200.000041
<input checked="" type="checkbox"/> Adjustment	Average reading of indicator	99.9998	199.9998
	Standard deviation	0.00006	0.00007

Unit :	Range :	<input type="checkbox"/> Before adjustment	<input type="checkbox"/> After adjustment
	Nominal value		
<input type="checkbox"/> No adjustment	Standard weight		
<input type="checkbox"/> Adjustment	Average reading of indicator		
	Standard deviation		

Certificate No. : 23-148800  
Sample Code : 23-56200-002

## REPORT OF CALIBRATION

## Result of Calibration

## 2. Sensitivity or value of a scale division

Change in the output variable of a measuring instrument divided by the associated change in the input variable.

Unit : g

Range : 220

Range : -

Test Point	Sensitivity, S	Test Point	Sensitivity, S
0	0.7980	-	-
100	0.8978	-	-
200	0.8978	-	-

## 3. Departure of indication from nominal value, Linearity

Unit : g

Nominal Value	Standard Value	Average Reading of Indicator	Correction Value	Expanded Uncertainty	Coverage Factor (k)
Unload	0.0000000	0.0000	0.0000	0.000086	2.00
0.01	0.0100025	0.0100	0.0000	0.000086	2.00
0.1	0.1000019	0.1000	0.0000	0.000087	2.00
1	1.0000125	1.0000	0.0000	0.000087	2.00
2	2.0000089	2.0000	0.0000	0.000087	2.00
5	5.0000208	5.0001	-0.0001	0.000088	2.00
10	10.000004	10.0000	0.0000	0.000090	2.00
20	20.000030	20.0000	0.0000	0.000093	2.00
50	50.000014	50.0000	0.0000	0.00011	2.00
100	100.000042	100.0000	0.0000	0.00016	2.00
200	200.000041	200.0000	0.0000	0.00028	2.00

The result expanded uncertainty of measurement  $U$  is stated as the standard uncertainty of measurement multiplied by the coverage factor  $k$ , which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty of measurement has been determined in accordance with UKAS M3003.

Certificate No. : 23-148800  
Sample Code : 23-56203-002


## REPORT OF CALIBRATION

## Result of Calibration :

## 4. Eccentric or off-centre loading

Deviation of the measurement value through off-center (eccentric) loading. The corner load increases with the weight of the load and its removal from the center of the pan support.

Weighing pan	<input checked="" type="radio"/> Circle <input type="radio"/> Triangular <input type="radio"/> Rectangular	Test weight : 100 Unit : g
Range	220	
Position	Reading of indicator	Reading of indicator
1	100.0000	-
2	100.0000	-
3	100.0000	-
4	99.9999	-
5	100.0000	-
6	100.0000	-
Maximum difference	0.0001	-

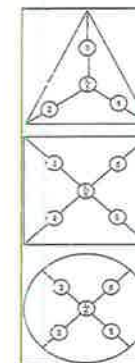

## Condition of Calibration

1. Calibration Method : WI-CL-004 base on UKAS LAB 14: 2019
2. This result of calibration was found accurate as shown on date and place of calibration only.
3. Condition of Calibration item: Normal

4. This certification is traceable to the International System of Unit maintained at : \*

\* Through the reference standard laboratory of Asia Medical and Agricultural Laboratory and Research Center Public Company Limited (Instrument number 1)

## 5. Reference standard instrument :

Instrument	Class	ID No.	Certificate No.	Due Date
1) STANDARD WEIGHT 1 mg to 1 kg	E2	LB-WE-79	23-105642	10 September 2024

End of Report

6. Ambient conditions	Min	Max
Temperature (°C)	24.4	24.8
Relative Humidity (%Rh)	39.9	41.1
Air pressure (hPa)	1012.2	1012.8

**BOD INCUBATOR**

**Model : TC445S**

**Serial No. : 0223/007275**

SK

S K SALES AND SERVICE CO.,LTD.  
194/56, 194/57 Thakham Rd. Samoe Dam  
Bang Khun Thien Bangkok 10150  
Tel. : 02-417-2144 Fax : 02-417-2155



## Certificate of Calibration

Reference No. : C03190/2309-025 Certificate No. : S2309-3014  
Customer : Eastern Thai Consulting 1992 Co.,Ltd. Page 1 of 2  
683 Moo 11, Sukhaphiban 8, Tambol Nongkham,  
Siracha District, Chonburi 20230, Thailand  
Equipment : Incubator  
Manufacturer : Lovibond  
Model : TC445S  
Serial No. : 0223/007275  
ID No. :  
Received Date : 15 September 2023  
Calibrated Date : 15 September 2023  
Issued Date : 18 September 2023  
Environment :

	Minimum Value	Maximum Value
Ambient Temperature ( °C )	27.5	28.1
Relative Humidity ( % RH )	57	58
AC Line Voltage ( VAC )	224	226
Place Of Calibration	Production Line	
Calibrated by	Mr. Teerasak Chalyaporn	

### Calibration Method

In-house method : SK-WI-23 base on Thai Laboratory Accreditation Scheme Publication Reference G-20

### Condition of this result of calibration

#### 1. Reference standard instrument

Instrument	Serial No.	Certificate No.	Due Date
1) Data acquisition/Switch unit	MY44047397	L2305-268	4 November 2023
2) Multiplexer Module	MY41105123	L2305-268	4 November 2023

2. This result of calibration was found accurate as shown on date and place of calibration only

3. This certificate can be traceable to International System of Unit :

- Through Thailand Institute of Scientific And Technological Research (TISTR)

Approved by

☒ Mr. Suphachai Saksri ☐ Mr. Phayak Toolit ☐ Miss Tantaraporn Pettong

The reported uncertainty is based on a standard uncertainty multiplied by a coverage factor  $k = 2.0$  ,providing a level of confidence level of approximately 95 %

This certificate may not be reproduced other than in full except with the prior written approval of the S K Sales And Service Company Limited

Certificate No. : S2309-3014

Page 2 of 2

Table1 General Information

Working Area ( W*L*H )	60 *56 *145 cm
Fresh Air	OFF

Table2 Chamber Performance


Setting Temperature ( °C )	Average Indicating Temperature ( °C )	Measured Stability ( ± °C )	Measured Uniformity ( °C )	Overall Variation ( °C )
20.0	20.0	0.37	0.64	0.98

Table3 Temperature Distribution

Setting Temperature ( °C )	Average Standard Reading ( °C )									Uncertainty ( ± °C )
	No. 1	No. 2	No. 3	No. 4	No. 5	No. 6	No. 7	No. 8	No. 9	
20.0	19.52	19.40	19.70	19.43	19.33	19.39	19.45	19.58	19.67	0.55

Resolution : 0.1 ( °C )

\* Probe No. 9 is Reference Probe



Notes : 1. The temperature stability is the one-half of greatest maximum difference of measured temperatures at any one probe.

2. The temperature uniformity is the maximum difference of measured temperatures between of any probes and the measured temperature at the reference location which are observed at same time

3. Overall variation is the difference of maximum and minimum measured temperatures throughout observation time.

4. The reported uncertainty of measurement were excluded Uniformity and Stability

\*\* End of Calibration Report \*\*

COPY

COPY

**BOD INCUBATOR**

**ID No. : LABE 19/5**





Page 1 of 3

## CERTIFICATE OF CALIBRATION

Certificate No. : 23-040768  
Sample Code : 23-16178-002

Customer : EASTERN THAI CONSULTING 1992 CO., LTD.  
683 Moo 11, Sukhapiban 8 Rd., Nongkham,  
Sriracha, Chonburi 20230

Location of Calibration : EASTERN THAI CONSULTING 1992 CO., LTD.  
(Laboratory)

Equipment : Temperature controlled enclosures (Incubator)

Manufacturer : Lovibond Model : Tc445S

Serial No. : 0520/005227 ID No. : LABE 19/5

Date of Receipt : 21 April 2023 Date of Calibration : 21 April 2023

## Condition of Calibration

1. Environment
- |                           |   |         |           |   |         |           |
|---------------------------|---|---------|-----------|---|---------|-----------|
| 1.1 Ambient temperature   | : | Maximum | 36.1 °C   | : | Minimum | 34.5 °C   |
| 1.2 Relative humidity     | : | Maximum | 51.8 %    | : | Minimum | 49.3 %    |
| 1.3 Line voltage supplied | : | Maximum | 224.7 VAC | : | Minimum | 221.9 VAC |

## 2. Calibration method

TLAS-G-20: Guidelines for calibration and checks of temperature controlled enclosures.

## 3. Reference standard instrument

Instrument	ID No.	Certificate No.	Due Date
Data Acquisition With Sensor (RTD-Pt100)	LB-DA-08 (RTD-239 to RTD-247)	22-077888	09 August 2023

## 4. This certificate is traceable to the international system of unit (SI Unit).

The measurement is traceable to Asia Medical and Agricultural Laboratory and Research Center Public Company Limited.

## 5. This result of calibration was found accurate as shown on date and place of calibration only.

## 6. Condition of calibration item : Normal

Calibrated by Mr. Sarawoot Thammo  
Scientist

Issue date 24 April 2023

Approved by

(Mr. Somchai Neampunt)

Signed for Director

COPY

The uncertainties are for a confidence probability of approximately 95%.

The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Asia Medical and Agricultural Laboratory and Research Center Public Company Limited (AMARC).

NSC-TISI-TIS17025  
CALIBRATION 0152

Page 2 of 3

## REPORT OF CALIBRATION

Certificate No. : 23-040768  
Sample Code : 23-16178-002

## Results of Calibration

Resolution : 0.1 °C

## 1. Reporting of Temperature

Calibration point (°C)	UUC* setting (°C)	UUC* reading (°C)	Measured temperature at each positions (°C)									Uncertainty ± (°C)	Coverage factor k
			# 1	# 2	# 3	# 4	# 5	# 6	# 7	# 8	# 9 <sup>Ref</sup>		
20	20.0	20.0	20.06	19.92	19.96	19.89	19.93	20.08	19.97	19.79	19.86	0.42	2.00

## 2. Characterization results

Calibration point (°C)	Stability ± (°C)	Uniformity (°C)	Overall variation (°C)
20	0.32	0.37	0.85

## Notes

- UUC\* = Unit Under Calibration

COPY

**Hot Air Oven**

**Model : UM 400**

**Serial No. : 900982**

## CERTIFICATE OF CALIBRATION

Certificate No. : 24-001944  
Sample Code : 24-00963-001Customer : EASTERN THAI CONSULTING 1992 CO., LTD.  
683 Moo 11, Sukhapibarn 8 Rd., Nongkham,  
Sriracha, Chonburi 20230Location of Calibration : EASTERN THAI CONSULTING 1992 CO., LTD.  
(Hot Lab)

Equipment : Temperature controlled enclosures (Hot air oven)

Manufacturer : Memmert Model : UM 400

Serial No. : 900982 ID No. : LABE 17/1

Date of Receipt : 09 January 2024 Date of Calibration : 09 January 2024

## Condition of Calibration

1. Environment

1.1 Ambient temperature	: Maximum	30.6 °C	: Minimum	29.2 °C
1.2 Relative humidity	: Maximum	57.5 %	: Minimum	46.4 %
1.3 Line voltage supplied	: Maximum	229.5 VAC	: Minimum	222.5 VAC

## 2. Calibration method

TLAS-G-20: Guidelines for calibration and checks of temperature controlled enclosures.

## 3. Reference standard instrument

Instrument	ID No.	Certificate No.	Due Date
Data Acquisition With Sensor (RTD-Pt100)	LB-DA-10 (RTD-257 to RTD-265)	23-066256	29 June 2024

## 4. This certificate is traceable to the international system of unit (SI Unit).

The measurement is traceable to Asia Medical and Agricultural Laboratory and Research Center Public Company Limited.

## 5. This result of calibration was found accurate as shown on date and place of calibration only.

## 6. Condition of calibration item : Normal

Calibrated by Mr. Sarawoot Thammo  
Scientist

Approved by

(Mr. Somchai Nearnpunt)

Signed for Director

Issue date 09 January 2024

The uncertainties are for a confidence probability of approximately 95%.

The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Asia Medical and Agricultural Laboratory and Research Center Public Company Limited (AMARC).

## REPORT OF CALIBRATION

Certificate No. : 24-001944  
Sample Code : 24-00963-001

## Results of Calibration

Resolution : 0.1 °C

## 1. Reporting of Temperature

Calibration point (°C)	UUC* setting (°C)	UUC* reading (°C)	Measured temperature at each positions (°C)									Uncertainty ± (°C)	Coverage factor k
			# 1	# 2	# 3	# 4	# 5	# 6	# 7	# 8	# 9 <sup>Ref</sup>		
60	60.0	60.0	60.04	59.90	59.81	59.84	59.47	59.91	60.08	59.98	59.87	0.25	2.00
85	85.0	85.0	86.07	85.75	85.58	85.62	84.69	85.83	86.28	85.94	85.77	0.34	2.00

## 2. Characterization results

Calibration point (°C)	Stability ± (°C)	Uniformity (°C)	Overall variation (°C)
60	0.11	0.49	0.80
85	0.09	1.13	1.72

## Notes

- UUC\* = Unit Under Calibration



## REPORT OF CALIBRATION

Certificate No. : 24-001944

Sample Code : 24-00963-001

## Results of Calibration

## Notes

1. Sensor installation locations
  - 1.1 All sensors at any corners or walls should be positioned 5 cm (a x b x c) from the wall.
  - 1.2 The reference sensor is preferably located of the geometric center of the chamber.
2. Interior dimensions approx of chamber :  
W = 40 cm ; D = 28 cm ; H = 39 cm
3. Air valve or fresh air level : Off
4. Fan level : Open
5. The quoted uncertainty includes "Stability of chamber and loading effect in chamber at 20% of uniformity".
6. Uniformity - the maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time.
7. Stability - one-half of the greatest maximum difference of measured temperatures at any one sensor.
8. Overall variation - the difference of the maximum and the minimum measured temperatures throughout observation time.
9. UUC\* reading - the average reading of indicating device that forms the integral part of the enclosure.
10. Calibration results without adjustment.

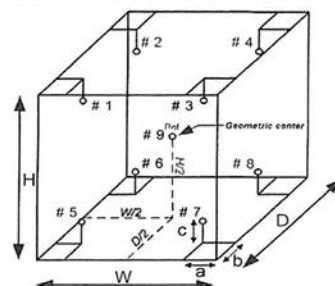


Figure: Example of sensor  
installation Positions

The result expanded uncertainty of measurement  $U$  is stated as the standard uncertainty of measurement multiplied by the coverage factor  $k$ , which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty of measurement has been determined in accordance with UKAS M3003.

- End of Report -

**COPY**

**LIQUID IN GLASS THERMOMETER**

**Model : Total Immersion**

**Serial No. : 43560**



QUALITY CALIBRATION CO.,LTD.  
235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160  
Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584  
www.qcalibration.com



CERTIFICATE No : 23T10864  
REFERENCE No : 71117-1

PAGE : 1 OF 2

## Certificate of Calibration

EQUIPMENT : LIQUID IN GLASS THERMOMETER  
MANUFACTURER : PRECISION  
MODEL : 0 °C TO 100 °C  
SERIAL No : 43560  
ID No : LABE 16/1  
RESOLUTION : 0.1 °C  
TYPE : TOTAL IMMERSION  
CONDITION AS RECEIVED : USED ITEM  
SUBMITTED BY : EASTERN THAI CONSULTING 1992 CO., LTD.  
683 MOO 11, SUKHAPIBAN 8 ROAD, NONGKHAM,  
SRIRACHA, CHONBURI 20230

CALIBRATED BY : CHARUKIT L.  
CALIBRATION DATE : 09-Nov-23  
APPROVED BY : PONGSAK J.  
ISSUED DATE : 09-Nov-23  
RECEIVED DATE : 02-Nov-23

**COPY**

THIS CERTIFICATE MAY NOT BE REPRODUCED OTHER THAN IN FULL EXCEPT WITH THE PRIOR WRITTEN APPROVAL OF  
QUALITY CALIBRATION CO., LTD.



QUALITY CALIBRATION CO.,LTD.  
235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160  
Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584  
www.qcalibration.com

CERTIFICATE No : 23T10864

PAGE : 2 OF 2

## Calibration Report

EQUIPMENT : LIQUID IN GLASS THERMOMETER  
MANUFACTURER : PRECISION  
MODEL : 0 °C TO 100 °C  
ID No : LABE 16/1  
RESOLUTION : 0.1 °C  
RECEIVED DATE : 02-Nov-23  
AMBIENT TEMPERATURE : 23 °C ± 3 °C  
SERIAL NUMBER : 43560  
TYPE : TOTAL IMMERSION  
CALIBRATION DATE : 09-Nov-23  
RELATIVE HUMIDITY : 50 %RH ± 20 %RH

### CONDITION OF THIS RESULTS OF CALIBRATION

- THIS INSTRUMENT WAS CALIBRATED BASED ON ASTM E77:1992 BY COMPARISON WITH STANDARD PLATINUM RESISTANCE THERMOMETER (SPRT) INTO LIQUID BATH TEMPERATURE CONTROLLER. THE TEMPERATURE SCALE USED WAS BASED ON ITS-90.
- REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) STANDARD THERMOMETER	1502	77964	23T3927	08-Mar-24
2) SPRT PROBE	5614	636636	23T3927	08-Mar-24
3) PRECISION BATH	7320	A21105	22T13199	14-Dec-23
4) PRECISION BATH	CTR-40	A68155	22T13198	09-Dec-23
5) PRECISION BATH	6045	3C023	22T13200	19-Dec-23
- THE CERTIFICATE IS VALID FOR THE ITEM CALIBRATED AS SHOWN ON THE DATE AND PLACE OF CALIBRATION ONLY.
- THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.
- THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-  
- NATIONAL INSTITUTE OF METROLOGY (THAILAND).

### RESULT OF CALIBRATION : WITHOUT ADJUSTMENT

STANDARD READING (°C)	UUC* READING (°C)	IMMERSION DEPTH (mm)	CORRECTION (°C)	EMERGENT STEM TEMPERATURE (°C)	UNCERTAINTY OF MEASUREMENT (±°C)
0.009	0.0	60	0.0090	N/A	0.26
25.01	25.0	165	0.0050	N/A	0.26
50.00	50.0	275	0.0040	N/A	0.26
99.991	100.0	360	-0.009	29.3	0.26

### UUC\* : UNIT UNDER CALIBRATION

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR k=2, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.  
END OF CALIBRATION REPORT

**COPY**



**pH Meter**

**Model : SevenCompact S220**

**Serial No. : B448305208**



## CERTIFICATE OF CALIBRATION

Page 1 of 3

Supersede to Calibration Certificate No. 24-001949

Certificate No. : 24-001949/1

Sample Code : 24-00963-006

Customer : EASTERN THAI CONSULTING 1992 CO., LTD.

683 Moo 11, Sukhapibarn 8 Rd., Nongkham,  
Sriracha, Chonburi 20230Location of Calibration : EASTERN THAI CONSULTING 1992 CO., LTD.  
(Laboratory)

Equipment : pH Meter

Manufacturer : METTLER TOLEDO

Model : SevenCompact S220

Serial No. : B448305208

ID No. : LABE 11/4

Date of Receipt : 09 January 2024

Date of Calibration : 09 January 2024

## Condition of Calibration

## 1. Environment

1.1 Ambient temperature : 22.4 ± 0.2 °C 1.2 Relative humidity : 56.4 % ± 2.1 %

## 2. Calibration method

In house method WI-CL-019: based on direct measurement by using standard voltage calibrator and using certified reference material (CRM).

## 3. Reference standard / Certified reference material

Instrument	ID No.	Certificate No.	Due Date
3.1 Voltage Calibrator	LB-AMC-01	23E3244	03 October 2024
3.2 Digital Thermometer	LB-TH-33	23-098974	25 August 2024
Certified Reference Material	Lot. No.	Ref No.	Expire Date
3.3 Buffer Solution pH 4.008	919273	PH216.L5	24 September 2025
3.4 Buffer Solution pH 6.986	941727	PH107.L5	06 November 2024
3.5 Buffer Solution pH 9.997	919278	PH220.L5	24 September 2024

## 4. This certificate is traceable to the international system of unit (SI Unit).

4.1 Instrument No. 3.1 through Technology Promotion Association (Thailand-Japan).

4.2 Instrument No. 3.2 through Asia Medical and Agricultural Laboratory and Research Center Public Company Limited.

4.3 Buffer Solution No. 3.3 and No. 3.5 traceable to CPA chem (through primary measurement method-Harned cell using calibrated thermometer, barometer, and nanovoltmeter Accredited laboratory ISO/IEC 17025 and ISO/IEC 17034).

4.4 Buffer Solution No. 3.4 traceable to CPA chem (CPA RefN HARNED CELL LotN 61275737; CPA RefN HARNED CELL LotN 61273986 Accredited laboratory ISO/IEC 17025 and ISO/IEC 17034).

## 5. This result of calibration was found accurate as shown on date and place of calibration only.

## 6. Condition of calibration item : Normal

Calibrated by Mr. Nuttaput Timula

Approved by

(Mr. Sornchai Neampunt)

Scientist

Signed for Director

Issue date 31 January 2024

The uncertainties are for a confidence probability of approximately 95%.

The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Asia Medical and Agricultural Laboratory and Research Center Public Company Limited (AMARC).



## REPORT OF CALIBRATION

Page 2 of 3

Supersede to Calibration Certificate No. 24-001949

Certificate No. : 24-001949/1

Sample Code : 24-00963-006

Equipment : pH Meter Resolution : 0.01 pH ; 0.1 mV ; 0.1 °C  
Manufacturer : METTLER TOLEDO Model : SevenCompact S220  
Serial No. : B448305208 ID No. : LABE 11/4  
Range : -2.000 pH to 20.000 pH ; ± 2000.0 mV ; -5.0 °C to 130.0 °C

## Results of Calibration

## Part 1. DC Voltage measurement

pH Meter Serial No. : B448305208

Nominal Value	Applied DC Voltage	Average indicator reading		Uncertainty	Coverage factor
		mV	pH		
0	414.113	413.9	0.00	± 0.083	2.00
4	177.477	177.4	4.00	± 0.083	2.00
7	0.000	0.1	7.00	± 0.083	2.00
10	-177.477	-177.3	10.00	± 0.083	2.00
14	-414.113	-413.8	14.00	± 0.083	2.00

## Part 2. Performance of Electrode system

Electrode Manufacturer : METTLER TOLEDO Model : InLab Expert Pro-ISM

Electrode Serial No. : 2453982

Three-Point Calibration at pH4, pH7 and pH10 Percent Slope : 98.3

Standard Buffer Solution	Average indicator reading		Error Value	Uncertainty	Coverage factor
	pH	mV			
pH (@ 25 °C)			pH	pH	k
4.008	4.01	182.1	0.002	± 0.010	2.00
6.986	7.00	7.8	0.014	± 0.011	2.00
9.997	10.01	-167.2	0.013	± 0.011	2.00

The result expanded uncertainty of measurement  $U$  is stated as the standard uncertainty of measurement multiplied by the coverage factor  $k$ , which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty of measurement has been determined in accordance with UKAS M3003.

NSC-TISI-TIS17025  
CALIBRATION 0152

Page 3 of 3

## REPORT OF CALIBRATION

Supersede to Calibration Certificate No. 24-001949

Certificate No. : 24-001949/1

Sample Code : 24-00963-006

Equipment : pH Meter (Digital Thermometer with sensor)

## Thermometer readout

Manufacturer : METTLER TOLEDO Model : SevenCompact S220  
 Serial No. : B448305208 ID No. : LABE 11/4  
 Resolution : 0.1 °C Range : -5.0 °C to 130.0 °C

## Thermometer sensor

Manufacturer : METTLER TOLEDO Model : InLab Expert Pro-ISM  
 Serial No. : 2453982 ID No. : N/A

## Condition of Calibration

1. Environment 1.1 Ambient temperature : 22.6 °C ± 0.1 °C  
 1.2 Relative humidity : 55.1 % ± 3.3 %

## 2. Calibration method

- 2.1 The calibration use in house method WI-CL-021 : by comparison with standard thermometer  
 2.2 The calibration by comparison unit under calibration (UUC) to the standard thermometer in a calibration bath at the controlled temperature.  
 2.3 The temperature scale in use of this laboratory is the international temperature scale of 1990 (ITS-90).

## 3. Reference standard instrument

Instrument	Model	ID. No.	Certificate No.	Due date
3.1 Resistance Thermometer	PT-100	RTD-90	23-098974	25 August 2024
3.2 Thermometer Readout	GT-11	LB-TH-33	23-098974	25 August 2024

## 4. This certificate is traceable to the international system of unit (SI Unit).

Asia Medical and Agricultural Laboratory and Research Center Public Company Limited (Accreditation Under TLAS Laboratory Calibration No.0152)

## 5. This result of calibration was found accurate as shown on date and place of calibration only.

6. Condition of Calibration item : Normal

## Results of Calibration

Calibration point °C	Average of standard reading °C	Unit under calibration			Expanded uncertainty °C	Coverage factor k
		Immersion depth mm	Average reading °C	Correction value °C		
25	25.000	120	25.0	0.000	± 0.14	2.00

## Notes

- Calibration results without adjustment

The result expanded uncertainty of measurement  $U$  is stated as the standard uncertainty of measurement multiplied by the coverage factor  $k$ , which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty of measurement has been determined in accordance with UKAS M3003

- End of report -

**COPY**

**STANDARD WEIGHT 50 g**



Certificate No. : 22-052238  
Sample Code : 22-19150-003

## CERTIFICATE OF CALIBRATION

Customer : EASTERN THAI CONSULTING 1992 CO., LTD.  
683 Moo 11, Sukhapiban 8 Rd., Nongkham,  
Sriracha, Chonburi 20230

Location of Calibration : Asia Medical and Agricultural Laboratory and Research Center Public Company Limited  
(Calibration Laboratory)

Equipment : Standard Weight 50 g

Manufacturer : METTLER TOLEDO

Class : F1

Serial No. : N/A

ID No. : LABE 10/1

Date of Receipt : 18 May 2022

Date of Calibration : 30 May 2022

Calibrated by : Mr. Somwang Sangdee  
Scientist

Approved by : ( Mr. Somchai Neampunt )  
Signed for Director

Issue date : 31 May 2022

The uncertainties are for a confidence probability of approximately 95%.

The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Asia Medical and Agricultural Laboratory and Research Center Public Company Limited (AMARC).



Certificate No. : 22-052238  
Sample Code : 22-19150-003

## REPORT OF CALIBRATION

Equipment : Standard Weight 50 g  
Manufacturer : METTLER TOLEDO  
Class : F1  
Serial No. : N/A  
ID No. : LABE 10/1

Result of Calibration : ☒ Without adjustment ☐ Adjustment

Conventional value of the result of weighing in air. For a weight taken at a reference temperature ( $t_{ref}$ ) of 20°C, the conventional mass is the mass of a reference weight of a density ( $\rho_{ref}$ ) of 8000 kg.m<sup>-3</sup> which it balances in air of a reference density ( $\rho_0$ ) of 1.2 kg.m<sup>-3</sup>

Description	Deviation	Conventional	Expanded	Maximum	ID No.
		Mass	Uncertainty	Permissible Error	
	(mg)		(mg)	± (mg)	
50 g	-0.324	49.999676 g	0.10	0.30	LABE 10/1

The result expanded uncertainty of measurement  $U$  is stated as the standard uncertainty of measurement multiplied by the coverage factor  $k = 2.0$ , which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty of measurement has been determined in accordance with UKAS M3003

COPY

Certificate No. : 22-052238

Sample Code : 22-19150-003

Page 3 of 3

## REPORT OF CALIBRATION

## Condition of Calibration:

1. Ambient Conditions : Temperature  $20^{\circ}\text{C} \pm 1.5^{\circ}\text{C}$ , Relative humidity  $50\% \pm 10\%$  and air density  $1.20 \text{ kg/m}^3$ 

2. Calibration Method : Direct comparison weighing according to OIML R111-1 : 2004(E)

3. Reference standard instrument

Instrument	Class	ID No.	Certificate No.	Due Date
1) Standard Weight 1 mg to 1 kg	E2	LB-WE-79	21-079366	22 September 2022

4. This certification is traceable to the International System of Unit maintained at : -

Asia Medical and Agricultural Laboratory and Research Center Public Company Limited

(Instrument number 1).

5. Condition of Calibration item: Normal

## 6. Description of Calibrated Item :

Type and Nominal Value :	Standard Weight 50 g
Shape :	Cylindrical weight with knob
Material :	Stainless steel
Case :	Wooden Box
Comments :	Recalibration

- End of Report -

COPY



**STANDARD WEIGHT 100 g**



Certificate No. : 22-052239  
Sample Code : 22-19150-004

## CERTIFICATE OF CALIBRATION

Customer : EASTERN THAI CONSULTING 1992 CO., LTD.  
683 Moo 11, Sukhapiban 8 Rd., Nongkham,  
Sriracha, Chonburi 20230

Location of Calibration : Asia Medical and Agricultural Laboratory and Research Center Public Company Limited  
(Calibration Laboratory)

Equipment : Standard Weight 100 g

Manufacturer : N/A

Class : N/A

Serial No. : N/A

ID No. : LABE 10/2

Date of Receipt : 18 May 2022

Date of Calibration : 30 May 2022

Calibrated by : Mr. Somwang Sangdee  
Scientist

Approved by

( Mr. Somchai Neampunt )

Signed for Director

Issue date : 31 May 2022

The uncertainties are for a confidence probability of approximately 95%.

The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Asia Medical and Agricultural Laboratory and Research Center Public Company Limited (AMARC).



Certificate No. : 22-052239  
Sample Code : 22-19150-004

## REPORT OF CALIBRATION

Equipment : Standard Weight 100 g  
Manufacturer : N/A  
Class : N/A  
Serial No. : N/A  
ID No. : LABE 10/2

### Result of Calibration :

☒ Without adjustment

☐ Adjustment

Conventional value of the result of weighing in air. For a weight taken at a reference temperature ( $t_{ref}$ ) of 20°C, the conventional mass is the mass of a reference weight of a density ( $\rho_{ref}$ ) of 8000 kg.m<sup>-3</sup> which it balances in air of a reference density ( $\rho_0$ ) of 1.2 kg.m<sup>-3</sup>

Description	Deviation	Conventional	Expanded	Maximum	ID No.
		Mass	Uncertainty	Permissible Error	
	(mg)		(mg)	± (mg)	
100 g	-0.171	99.999829 g	0.16	0.50	LABE 10/2

The result expanded uncertainty of measurement  $U$  is stated as the standard uncertainty of measurement multiplied by the coverage factor  $k = 2.0$ , which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty of measurement has been determined in accordance with UKAS M3003

COPY



Certificate No. : 22-052239

Sample Code : 22-19150-004

Page 3 of 3

## REPORT OF CALIBRATION

## Condition of Calibration

1. Ambient Conditions : Temperature  $20^{\circ}\text{C} \pm 1.5^{\circ}\text{C}$ , Relative humidity  $50\% \pm 10\%$  and air density  $1.18 \text{ kg/m}^3$ 

2. Calibration Method : WI-CL-007 base on OIML R 111-1 : 2004(E)

3. Reference standard instrument

Instrument	Class	ID No.	Certificate No.	Due Date
1) Standard Weight 1 mg to 1 kg	E2	LB-WE-79	21-079366	22 September 2022

4. This certification is traceable to the International System of Unit maintained at : -

Asia Medical and Agricultural Laboratory and Research Center Public Company Limited

( Instrument number 1).

5. Condition of Calibration item: Normal

## 6. Description of Calibrated Item :

Type and Nominal Value :	Standard Weight 100 g
Shape :	Cylindrical weight with knob
Material :	Stainless steel
Case :	Wooden Box
Comments :	Recalibration

- End of Report -

COPY

**STANDARD WEIGHT 50 g**



Certificate No. : 22-052237  
Sample Code : 22-19150-002

## CERTIFICATE OF CALIBRATION

Customer : EASTERN THAI CONSULTING 1992 CO., LTD.  
683 Moo 11, Sukhapiban 8 Rd., Nongkham,  
Sriracha, Chonburi 20230

Location of Calibration : Asia Medical and Agricultural Laboratory and Research Center Public Company Limited  
(Calibration Laboratory)

Equipment : Standard Weight 50 g

Manufacturer : N/A

Class : N/A

Serial No. : N/A

ID No. : LABE 10/4

Date of Receipt : 18 May 2022

Date of Calibration : 30 May 2022

Calibrated by : Mr. Somwang Sangdee  
Scientist

Approved by : ( Mr. Somchai Neampunt )  
Signed for Director

Issue date : 31 May 2022

The uncertainties are for a confidence probability of approximately 95%.

The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Asia Medical and Agricultural Laboratory and Research Center Public Company Limited (AMARC).



Certificate No. : 22-052237  
Sample Code : 22-19150-002

## REPORT OF CALIBRATION

Equipment : Standard Weight 50 g  
Manufacturer : N/A  
Class : N/A  
Serial No. : N/A  
ID No. : LABE 10/4

### Result of Calibration :

☒ Without adjustment

☐ Adjustment

Conventional value of the result of weighing in air. For a weight taken at a reference temperature ( $t_{ref}$ ) of 20°C, the conventional mass is the mass of a reference weight of a density ( $\rho_{ref}$ ) of 8000 kg.m<sup>-3</sup> which it balances in air of a reference density ( $\rho_0$ ) of 1.2 kg.m<sup>-3</sup>

Description	Deviation	Conventional Mass	Expanded Uncertainty	Maximum Permissible Error	ID No.
	(mg)		(mg)	± (mg)	
50 g	-0.111	49.999889 g	0.10	0.30	LABE 10/4

The result expanded uncertainty of measurement  $U$  is stated as the standard uncertainty of measurement multiplied by the coverage factor  $k = 2.0$ , which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty of measurement has been determined in accordance with UKAS M3003

COPY

Certificate No. : 22-052237  
Sample Code : 22-19150-002

Page 3 of 3

## REPORT OF CALIBRATION

### Condition of Calibration

1. Ambient Conditions : Temperature  $20^{\circ}\text{C} \pm 1.5^{\circ}\text{C}$ , Relative humidity  $50\% \pm 10\%$  and air density  $1.18 \text{ kg/m}^3$
2. Calibration Method : WI-CL-007 base on OIML R 111-1 : 2004(E)
3. Reference standard instrument

Instrument	Class	ID No.	Certificate No.	Due Date
1) Standard Weight 1 mg to 1 kg	E2	LB-WE-79	21-079366	22 September 2022

4. This certification is traceable to the International System of Unit maintained at : -

Asia Medical and Agricultural Laboratory and Research Center Public Company Limited

( Instrument number 1).

5. Condition of Calibration item: Normal

### 6. Description of Calibrated Item :

Type and Nominal Value :	Standard Weight 50 g
Shape :	Cylindrical weight with knob
Material :	Stainless steel
Case :	Wooden Box
Comments :	Recalibration

- End of Report -



COPY



**UV/VIS SPECTROPHOTOMETER**

**Model : UV - 1800**

**Serial No. : A11635101643 CD**



**Bara Scientific Co., Ltd.**  
968 U Chu Liang Building Floor7 Rama4 Road  
Silom Bangrak Bangkok Thailand 10500  
Tel : 02-6324300 Fax : 02-6375496-7  
www.barascientific.com



# Certificate of Calibration

Number of Page(s) 1 of 3

**Certificate No.** BSCC-UV-152/23  
**Equipment** UV/Vis Spectrophotometer  
**Model** UV-1800  
**Manufacturer** Shimadzu  
**Serial No.** A11635101643 CD  
**ID No.** N/A  
**Date of receipt** 25 April 2023  
**Date of calibration** 25 April 2023  
**Date of issue** 27 April 2023

**Customer name** Eastern Thai Consulting 1992 Co.,Ltd  
**Address** 683 Moo 11, Sukkaphibarn 8 Rd., Nongkham, Sriracha, Chonburi 20230

**Temperature** (22.4-23.1) °C (On site)  
**Humidity** (44.5-45.2) %RH (On site)

**Equipment condition** Good Operation

**Calibration Location** Analysis Department

**Calibration Procedure** In-house method WI-UV-702-01 based on ASTM E275-01

**Traceability** Wavelength Accuracy is traceable to certificate No. 94780 and 94775  
Photometric Accuracy is traceable to certificate No. 94808 and 100147  
Stray Light is traceable to certificate No. 94791  
The above certificate are traceable to SI unit through Sarna Scientific Ltd.  
(UKAS accredited calibration laboratory NO. 0659)

**Calibrated by** Mr.Pannaphong Phanmekakul

Approved by

**Mr.Kanchit Choothep**  
Technical Manager

The above results are valid exclusively for the calibrated item(s) as mention in this report / certificate.  
Advertising the report / Certificate and publicity of the results are prohibited and also shall not be reproduced  
except in full, without written approval of the Bara Scientific Co., Ltd.



**Bara Scientific Co., Ltd.**  
968 U Chu Liang Building Floor7 Rama4 Road  
Silom Bangrak Bangkok Thailand 10500  
Tel : 02-6324300 Fax : 02-6375496-7  
www.barascientific.com



# Certificate of Calibration

**Certificate No.** BSCC-UV-152/23

**Number of Page(s)** 2 of 3

## Calibration Results:

### 1.Wavelength Accuracy

Certified Wavelength (nm)	UUC (nm)	Error (nm)	Uncertainty (±nm)
287.71	287.65	-0.06	0.18
445.82	445.80	-0.02	0.18
536.52	536.35	-0.17	0.18
741.02	740.99	-0.03	0.18
879.41	879.27	-0.14	0.18

### 2.Photometric Accuracy (UV)

Wavelength (nm)	Certified Absorbance (A)	UUC (A)	Error (A)	Uncertainty (±A)
235	0.0000 0.7311	0.0000 0.7313	0.0000 0.0002	0.0075 0.0075
257	CNR CNR	CNR CNR	CNR CNR	CNR CNR
313	CNR CNR	CNR CNR	CNR CNR	CNR CNR
350	0.0000 0.6306	0.0000 0.6314	0.0000 0.0008	0.0075 0.0075

\*CNR = Customer not request

The above results are valid exclusively for the calibrated item(s) as mention in this report / certificate.  
Advertising the report / Certificate and publicity of the results are prohibited and also shall not be reproduced  
except in full, without written approval of the Bara Scientific Co., Ltd.

# Certificate of Calibration

Certificate No. **BSCC-UV-152/23**

Number of Page(s) 3 of 3

## Calibration Results:

### 3. Photometric Accuracy (Visible)

Wavelength (nm)	Certified Absorbance (A)	UUC (A)	Error (A)	Uncertainty ( $\pm A$ )
420.0	0.0000	0.0000	0.0000	0.0042
	0.5488	0.5508	0.0020	0.0042
	0.7527	0.7535	0.0008	0.0042
	1.0756	1.0758	0.0002	0.0042
440.0	0.0000	0.0000	0.0000	0.0042
	0.5391	0.5406	0.0015	0.0042
	0.7355	0.7360	0.0005	0.0042
	1.0509	1.0501	-0.0008	0.0042
465.0	CNR	CNR	CNR	CNR
	CNR	CNR	CNR	CNR
	CNR	CNR	CNR	CNR
	CNR	CNR	CNR	CNR
546.1	0.0000	0.0000	0.0000	0.0042
	0.5045	0.5044	-0.0001	0.0042
	0.6884	0.6885	0.0001	0.0042
	0.9816	0.9808	-0.0008	0.0042
590.0	CNR	CNR	CNR	CNR
	CNR	CNR	CNR	CNR
	CNR	CNR	CNR	CNR
	CNR	CNR	CNR	CNR
635.0	0.0000	0.0000	0.0000	0.0042
	0.5183	0.5178	-0.0005	0.0042
	0.6864	0.6868	0.0004	0.0042
	0.9747	0.9739	-0.0008	0.0042

\*CNR = Customer not request

### 4. Stray Light\*

Standard cut-off wavelength (nm)	Unit Under Calibration(UUC)		
	Wavelength (nm)	Transmission (%T)	Absorbance (A)
200.75 $\pm$ 0.11nm	200.72	0.9630	2.0164

The Stray light transmission reference is less than 1.0%T and Stray light absorbance reference is greater than 2.00A  
\*Stray Light not NSC-ONSC Accredited.

The measurement uncertainty is base on a standard uncertainty multiplied by a coverage factor k=2 providing a level of confidence of approximately 95%.

\*\*\*End of Certificate\*\*\*

The above results are valid exclusively for the calibrated item(s) as mention in this report / Certificate.  
Advertising the report / Certificate and publicity of the results are prohibited and also shall not be reproduced except in full, without written approval of the Bara Scientific Co., Ltd.

**ANALYTICAL BALANCE (DU)**

**Model : XS205DU**


**Serial No. : 1126323724**

Mettler-Toledo (Thailand) Ltd.  
846/4 - 846/5846/4 - 846/5 Lasalle Rd., Bangna Tai  
Bangna District, Bangkok 10260  
+66 2723 0382  
MT-TH.ServiceSupport@mt.com



## Accuracy Calibration Certificate

### Customer

Company: EASTERN THAI CONSULTING 1992 CO., LTD.  
Address: 683 Moo 11, Sukhaphiban 8 Rd., Nong Kham  
City: Sriracha Contact: Sasiporn Nakin  
Zip / Postal: 20230  
State / Province: Chonburi  
Order Number:  0333319619

### Weighing Device

Manufacturer: Mettler Toledo Instrument Type: Weighing Instrument  
Model: XS205DU Asset Number: LABE 05/1  
Serial No.: 1126323724 Terminal Model: SAT  
Building: Laboratory Terminal Serial No.: 1126323724  
Floor: 1 Terminal Asset No.: N/A  
Room: Analytical Balance

Range	Max. Capacity	Readability (d)
1	81 g	0.00001 g
2	220 g	0.0001 g

### Procedure



Calibration Guidelines: EURAMET cg-18 v. 4.0 (11/2015)  
METTLER TOLEDO Work Instruction: CP/W002/20

This calibration certificate contains measurements for As Found calibration. No As Left calibration was performed because the device was not modified after As Found calibration. Therefore, results for As Left correspond to As Found.

The sensitivity/span of the weighing instrument was adjusted before calibration with a built-in weight.

In accordance with EURAMET cg-18 (11/2015), the test loads were selected to reflect the specific use of the weighing device or to accommodate specific calibration conditions.

	Temperature		Humidity	
As Found	Start: 25.7 °C	End: 25.8 °C	Start: 50.9 %	End: 50.6 %

As Found Calibration Date: 09-Dec-2024  
As Left Calibration Date: N/A  
Issue Date: 11-Dec-2024  
Calibrator:   
Somsak Sattanaco  
Approved Signatory:   
Sirachai P.  
Technical Manager / Head of Calibration Center


## Measurement Results

### Repeatability

Test Load: 70 g

	As Found	As Left
1	70.00004 g	N/A
2	70.00005 g	N/A
3	70.00004 g	N/A
4	70.00005 g	N/A
5	70.00006 g	N/A
6	70.00004 g	N/A
7	70.00005 g	N/A
8	70.00005 g	N/A
9	70.00006 g	N/A
10	70.00006 g	N/A

Standard Deviation	0.000008 g	N/A
--------------------	------------	-----

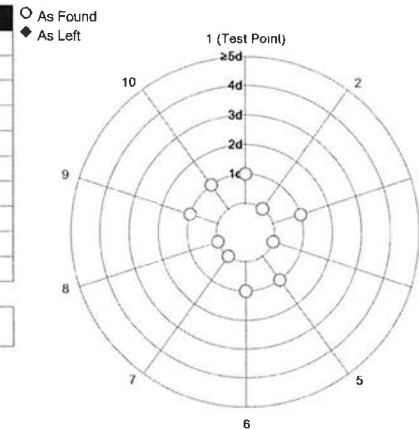

The "d" in the graph represents the readability of the range/interval in which the test was performed.


The results of this graph are based upon the absolute values of the differences from the mean value.

### Eccentricity

Test Load: 100 g

Position	As Found	As Left
1	100.0000 g	N/A
2	100.0000 g	N/A
3	100.0000 g	N/A
4	99.9999 g	N/A
5	100.0000 g	N/A

Maximum Deviation	0.0001 g	N/A
-------------------	----------	-----



As Found


The "d" in the graph represents the readability of the range/interval in which the test was performed.

Error of Indication

As Found

	Reference Value	Indication	Error of Indication	Expanded Uncertainty	k
1	0.00000 g	0.00000 g	0.00000 g	0.017 mg	2
2	0.01000 g	0.01000 g	0.00000 g	0.020 mg	2
3	0.10000 g	0.10000 g	0.00000 g	0.023 mg	2
4	1.00000 g	1.00000 g	0.00000 g	0.032 mg	2
5	4.99998 g	5.00000 g	0.00002 g	0.048 mg	2
6	10.00001 g	10.00001 g	0.00000 g	0.061 mg	2
7	19.99999 g	20.00001 g	0.00002 g	0.082 mg	2
8 *	50.00003 g	50.00005 g	0.00002 g	0.12 mg	2
9	100.00000 g	100.00000 g	0.00000 g	0.21 mg	2
10	150.00000 g	150.00000 g	0.00000 g	0.32 mg	2
11	200.00000 g	200.00000 g	0.00000 g	0.37 mg	2

\*The calculated uncertainty was replaced by the CMC (Calibration and Measurement Capabilities) value because the calculated uncertainty was smaller than the CMC value.

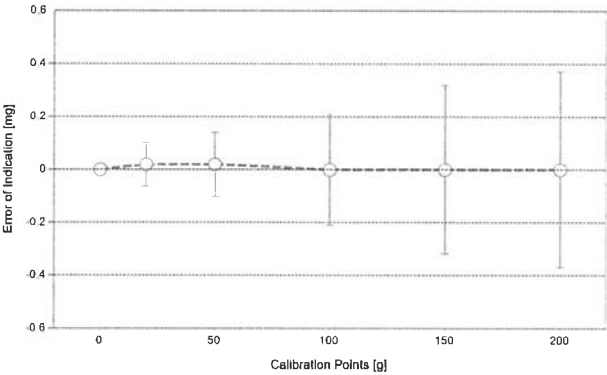

○ As Found

◆ As Left

For improved legibility of the graphics only increasing measurement points are shown and measurement points close to zero are not displayed.

The expanded measurement uncertainty is reported as the standard measurement uncertainty multiplied by the coverage factor k such that the coverage probability corresponds to approximately 95 %.

The user is responsible for maintaining environmental conditions and the settings of the weighing instrument when it was calibrated.  
The results of this calibration certificate relate only to the calibrated item.

Test Equipment

All weights used for metrological testing are traceable to national or international standards. The weights were calibrated and certified by an accredited calibration laboratory.

Weight Set 1: OIML E2

Weight Set No.: WS37 Date of Issue: 17-Jun-2024  
Certificate Number: 186753-1 Calibration Due Date: 20-Jan-2025

Weight Set 2: OIML E2

Weight Set No.: WS87 Date of Issue: 04-Jul-2023  
Certificate Number: 186520 Calibration Due Date: 02-Jan-2025

Thermo Hygrometer

Equipment No.: IN279 Date of Issue: 19-Jun-2024  
Certificate Number: SG-H-00577/67 Calibration Due Date: 17-Jun-2025

Remarks

FACT adjustment functionality activated  
Equipment condition: Good  
Next calibration according to customer's procedure  
Calibration data not decide by calibration laboratory

End of Accredited Section

The information below and any attachments to this calibration certificate are not part of the accredited calibration.



Measurement Uncertainty of the Weighing Instrument in Use

Stated is the expanded uncertainty with k=2 in use. The formula shall be used for the estimation of the uncertainty under consideration of the errors of indication. The value R represents the net load indication in the unit of measure of the device.

Temperature coefficient for the evaluation of the measurement uncertainty in use: 1.5 · 10<sup>-8</sup> / K  
Temperature range on site for the evaluation of the measurement uncertainty in use: 3 K


Linearization of Uncertainty Equation

Range		As Found		As Left
d	Max			
1	0.00001 g	81 g	U <sub>1</sub> = 0.018 mg + 0.00444 mg/g · R	N/A
2	0.0001 g	220 g	U <sub>2</sub> = 0.06 mg + 0.00439 mg/g · R	N/A

To optimize the stability of the linearization, besides of the zero load only increasing measurement points with a test load of 5% of the measurement range or larger are taken for the calculation of the linear equation.

Absolute and Relative Measurement Uncertainty in Use for Various Net Indications (Example)

Net Indication	As Found		As Left	
0.00220 g	0.018 mg	0.82%	N/A	N/A
0.02200 g	0.018 mg	0.082%	N/A	N/A
0.22000 g	0.019 mg	0.0086%	N/A	N/A
2.20000 g	0.028 mg	0.0013%	N/A	N/A
220.0000 g	1.0 mg	0.00047%	N/A	N/A

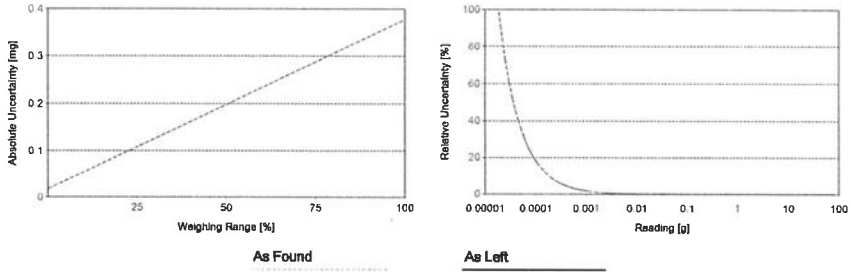

The weighing range shown in the absolute uncertainty graph refers to the first interval/range of the device.

GWP®  
Certificate



As Found



As Left



The weighing device meets the given process requirements.


The weighing device meets the given process requirements.

Tests Performed: ☒ As Found ☐ As Left ☒ No adjustments/modifications made. As Left results correspond to As Found.

Process Requirements

Weighing Tolerance: 1% | Smallest Net Weight: 0.01000 g | Safety Factor: 2

Safe Weighing Range

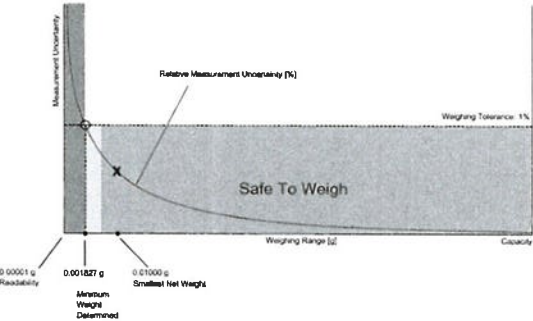

While the values in this graph reflect the actual calibration results, the measurement uncertainty curves are simply a visual representation. This graph reflects As Left testing, unless only As Found was performed.

## Minimum Weight

### As Found Minimum Weight Table

#### Range 1

Minimum weights for different weighing tolerances and safety factors					
Tolerance	Safety Factor				
	1	2	3	5	10
0.1%	0.018339 g	0.036842 g	0.055511 g	0.093358 g	0.191052 g
0.2%	0.009149 g	0.018339 g	0.027570 g	0.046156 g	0.093358 g
0.5%	0.003655 g	0.007316 g	0.010984 g	0.018339 g	0.036842 g
1%	0.001827 g	0.003655 g	0.005485 g	0.009149 g	0.018339 g
2%	0.000913 g	0.001827 g	0.002740 g	0.004569 g	0.009149 g
5%	0.000365 g	0.000730 g	0.001096 g	0.001827 g	0.003655 g

The minimum weight table applies to the fine range of the weighing device.

✓ Pass: The determined minimum weight meets the requirement for the smallest net weight.

### As Left Minimum Weight Table

#### Range 1

Minimum weights for different weighing tolerances and safety factors					
Tolerance	Safety Factor				
	1	2	3	5	10
0.1%	0.018339 g	0.036842 g	0.055511 g	0.093358 g	0.191052 g
0.2%	0.009149 g	0.018339 g	0.027570 g	0.046156 g	0.093358 g
0.5%	0.003655 g	0.007316 g	0.010984 g	0.018339 g	0.036842 g
1%	0.001827 g	0.003655 g	0.005485 g	0.009149 g	0.018339 g
2%	0.000913 g	0.001827 g	0.002740 g	0.004569 g	0.009149 g
5%	0.000365 g	0.000730 g	0.001096 g	0.001827 g	0.003655 g

The minimum weight table applies to the fine range of the weighing device.

✓ Pass: The determined minimum weight meets the requirement for the smallest net weight.

At these net minimum weight values, the measurement uncertainty of the weighing device is equal to or less than 1/1 (no safety factor), 1/2, 1/3, 1/5, or 1/10 of the required tolerance. The values are calculated with  $k = 2$  and based on the linear formula of the measurement uncertainty of the weighing device in use.

The safety factor for As Found is always 1. This implies no safety factor. As Found testing looks at the behavior of the instrument from the past until test occurred. For the past, it is necessary to know that the tolerance was met, but not the safety factor. The safety factor is a proactive measure to apply for future measurements.

#### Notes on minimum weight values in above table:

1. If "N/A" is shown above, no appropriate value could be calculated.
2. METTLER TOLEDO is not responsible for the definition of the process requirements.

COPY

## Measurement Results

### Results Summary

	Repeatability	Eccentricity	Error of Indication
As Found	✓	✓	✓
As Left	✓	✓	✓

✓ = Passed

✗ = Failed

⚠ = Safety Factor not met

### Repeatability

Test Load: 70 g

Tolerance	Control Limit	As Found		As Left	
		Std. Deviation	Result	Std. Deviation	Result
0.1%	0.000005 g	0.000008 g	✗	0.000008 g	✗
0.2%	0.000010 g		✓		⚠
0.5%	0.000025 g		✓		✓
1%	0.000050 g		✓		✓
2%	0.000100 g		✓		✓
5%	0.000250 g		✓		✓

The weighing tolerance is met if the standard deviation is less than or equal to the corresponding control limit.

### Eccentricity

Test Load: 100 g

Tolerance	Control Limit	As Found		As Left	
		Deviation	Result	Deviation	Result
0.1%	0.0500 g	0.0001 g	✓	0.0001 g	✓
0.2%	0.1000 g		✓		✓
0.5%	0.2500 g		✓		✓
1%	0.5000 g		✓		✓
2%	1.0000 g		✓		✓
5%	2.5000 g		✓		✓

The weighing tolerance is met if the deviation is less than or equal to the corresponding control limit.

COPY

Error of Indication

As Found

		Control limits for various weighing tolerances					
Reference Value	Error	0.1%	0.2%	0.5%	1%	2%	5%
0.00000 g	0.00000 g	N/A	N/A	N/A	N/A	N/A	N/A
19.99999 g	0.00002 g	0.01000 g	0.02000 g	0.05000 g	0.10000 g	0.20000 g	0.50000 g
50.00003 g	0.00002 g	0.02500 g	0.05000 g	0.12500 g	0.25000 g	0.50000 g	1.25000 g
100.0000 g	0.0000 g	0.0500 g	0.1000 g	0.2500 g	0.5000 g	1.0000 g	2.5000 g
150.0000 g	0.0000 g	0.0750 g	0.1500 g	0.3750 g	0.7500 g	1.5000 g	3.7500 g
200.0000 g	0.0000 g	0.1000 g	0.2000 g	0.5000 g	1.0000 g	2.0000 g	5.0000 g
Result		✓	✓	✓	✓	✓	✓

As Left

		Control limits for various weighing tolerances					
Reference Value	Error	0.1%	0.2%	0.5%	1%	2%	5%
0.00000 g	0.00000 g	N/A	N/A	N/A	N/A	N/A	N/A
19.99999 g	0.00002 g	0.01000 g	0.02000 g	0.05000 g	0.10000 g	0.20000 g	0.50000 g
50.00003 g	0.00002 g	0.02500 g	0.05000 g	0.12500 g	0.25000 g	0.50000 g	1.25000 g
100.0000 g	0.0000 g	0.0500 g	0.1000 g	0.2500 g	0.5000 g	1.0000 g	2.5000 g
150.0000 g	0.0000 g	0.0750 g	0.1500 g	0.3750 g	0.7500 g	1.5000 g	3.7500 g
200.0000 g	0.0000 g	0.1000 g	0.2000 g	0.5000 g	1.0000 g	2.0000 g	5.0000 g
Result		✓	✓	✓	✓	✓	✓

The weighing tolerance is met if the error (of indication) for each test point is less than or equal to the corresponding control limit for that particular weighing tolerance. Results at or close to the zero point cannot be assessed.

COPY

**ANALYTICAL BALANCE**

**Model : SECURA224-1S**

**Serial No. : 0036707137**



Certificate No. : 24-164695  
Sample Code : 24-67405-005

## CERTIFICATE OF CALIBRATION

Customer : EASTERN THAI CONSULTING 1992 CO., LTD.  
683 Moo 11, Sukhapibarn 8 Rd, Nongkham,  
Sriracha, Chonburi 20230

Location of Calibration : EASTERN THAI CONSULTING 1992 CO., LTD.  
(Analytical Balance Room)

Equipment : ELECTRONIC BALANCE

Manufacturer : SARTORIUS

Model : SECURA224-1S

Serial No. : 0036707137

ID No. : LABE 05/2

Date of Receipt : 19 December 2024

Date of Calibration : 19 December 2024

Calibrated by Mr. Thanadol Pholthep  
Scientist

Approved by (Mr. Nuttaput Timula)  
Signed for Director

Issue date 20 December 2024

The uncertainties are for a confidence probability of approximately 95%.

The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Asia Medical and Agricultural Laboratory and Research Center Public Company Limited (AMARC).



Certificate No. : 24-164695  
Sample Code : 24-67405-005

## REPORT OF CALIBRATION

Equipment : ELECTRONIC BALANCE  
Manufacturer : SARTORIUS  
Model : SECURA224-1S  
Capacity : Max 220 g  
Resolution : 0.0001 g  
Serial No. : 0036707137  
ID No. : LABE 05/2

## Result of Calibration

## 1. Test weight and repeatability of reading

Repeatability is a measure of the ability of a balance to supply the same result in repetitive weighings with one and the same load under the same measurement condition. The measurement of the repeatability must include both the balance specifications and the ambient (vibration, fluctuating air current/temperature/humidity, etc.) Operator handling of the balance is also included in the standard deviation.

Unit : g	Range : 220	<input type="checkbox"/> Before adjustment	<input type="checkbox"/> After adjustment
<input checked="" type="checkbox"/> No adjustment	Nominal value	100	200
<input type="checkbox"/> Adjustment	Standard weight	100.000016	200.000028
	Average reading of indicator	100.0000	200.0000
	Standard deviation	0.00005	0.00005
Unit : -	Range : -	<input type="checkbox"/> Before adjustment	<input type="checkbox"/> After adjustment
<input type="checkbox"/> No adjustment	Nominal value	-	-
<input type="checkbox"/> Adjustment	Standard weight	-	-
	Average reading of indicator	-	-
	Standard deviation	-	-



Certificate No. : 24-164695  
Sample Code : 24-67405-005

Page 3 of 4

## REPORT OF CALIBRATION

## Result of Calibration

## 2. Sensitivity or value of a scale division

Change in the output variable of a measuring instrument divided by the associated change in the input variable.

Unit : g

Range : 220

Range :

Test Point	Sensitivity, S	Test Point	Sensitivity, S
0	0.9998	-	-
100	0.9998	-	-
200	0.8998	-	-

## 3. Departure of indication from nominal value, Linearity

Unit : g

Nominal Value	Standard Value	Average Reading of Indicator	Correction Value	Expanded Uncertainty	Coverage Factor (k)
Unload	0.0000000	0.0000	0.0000	0.000094	2.01
0.01	0.0100015	0.0100	0.0000	0.000094	2.01
0.1	0.1000064	0.1000	0.0000	0.000094	2.01
1	1.0000017	1.0000	0.0000	0.000095	2.01
2	2.0000049	2.0000	0.0000	0.000095	2.01
5	5.0000012	5.0000	0.0000	0.000096	2.01
10	9.999992	10.0000	0.0000	0.000097	2.01
20	20.000042	20.0000	0.0000	0.00010	2.01
50	50.000046	50.0000	0.0000	0.00012	2.01
100	100.000016	100.0000	0.0000	0.00016	2.00
200	200.000028	200.0000	0.0000	0.00028	2.00

The result expanded uncertainty of measurement  $U$  is stated as the standard uncertainty of measurement multiplied by the coverage factor  $k$ , which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty of measurement has been determined in accordance with UKAS M3003.

Certificate No. : 24-164695  
Sample Code : 24-67405-005

Page 4 of 4


## REPORT OF CALIBRATION

## Result of Calibration :

## 4. Eccentric or off-centre loading

Deviation of the measurement value through off-center (eccentric) loading. The corner load increases with the weight of the load and its removal from the center of the pan support.

Weighing pan		
<input checked="" type="radio"/> Circle		
<input type="radio"/> Triangular		
<input type="radio"/> Rectangular		
Range	220	Test weight : 100
Position	Reading of indicator	Unit : g
1	99.9999	-
2	100.0001	-
3	99.9999	-
4	99.9998	-
5	99.9999	-
6	99.9999	-
Maximum difference	0.0002	-

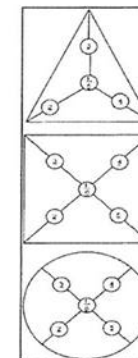

## Condition of Calibration

1. Calibration Method : WI-CL-004 base on UKAS LAB 14: 2019

2. This result of calibration was found accurate as shown on date and place of calibration only.

3. Condition of Calibration item: Normal

4. This certification is traceable to the International System of Unit maintained at : -

- Through the reference standard laboratory of Asia Medical and Agricultural Laboratory and Research Center Public Company Limited (Instrument number 1).

5. Reference standard instrument :

Instrument	Class	ID No.	Certificate No.	Due Date
1) STANDARD WEIGHT 1 mg to 1 kg	E2	LB-WE-78	24-097116	02 August 2025

- End of Report -

6. Ambient conditions	Min	Max
Temperature (°C)	25.0	25.4
Relative Humidity (%Rh)	39.8	41.0
Air pressure (hPa)	1011.0	1012.1

**ATOMIC ABSORPTION SPECTROPHOTOMETER**


**Model : Pin AAcle 900F**

**Serial No. : PFBS22080801**



### PinAAcle 900F Preventive Maintenance (PM)

Company Name:	EASTERN THAI CONSULTING		
Address (Instrument Location):	683 Moo 11 Nong Kham, Sri Racha, Chonburi 20230		
Serial Number:	PFBS2208081	PM Number:	1/2
Customer Name (if applicable):	K.Channarong	Telephone Number:	096-8761232
Customer Support Engineer Name:	Prasit	Service Order Number:	WO-03149105
Date PM Performed: (DD-MMM-YYYY)	22 APR 2025	Next PM Due Date: (DD-MMM-YYYY)	22 OCT 2025
Standard Labor Hours to Complete PM :		5 hours	

Part Number	Release	Publication Date	
09370145 Rev.9	A	January 2018	

#### Scope

The purpose of this PM is to ensure the continued functionality of the PinAAcle 900F by inspecting and replacing any worn or damaged parts. This service should only be performed by a trained representative of PerkinElmer.

The customer should save their method before the PM begins.

#### General Instructions:

The customer must provide the engineer operational data to demonstrate recent instrument performance prior to starting the PM.

Always check with the customer before making any changes that may affect the customer's analysis or calibration, including a current back-up of system software and/or data files.

The completed document should be signed by an authorized PerkinElmer and customer representative and left with the customer.

Update the PM sticker and instrument logbook as required.

#### Copyright Information

This document contains proprietary information that is protected by copyright. All rights are reserved.

No part of this publication may be reproduced in any form whatsoever or translated into any language without the prior, written permission of PerkinElmer, Inc.

Copyright © 2013 PerkinElmer, Inc.

#### Trademarks

Registered names, trademarks, etc. used in this document, even when not specifically marked as such, are protected by law. PerkinElmer is a registered trademark of PerkinElmer, Inc. All other trademarks and registered trademarks not owned by PerkinElmer, Inc. or its subsidiaries that are depicted herein are the property of their respective owners. Except as specifically set forth in its terms and conditions of sale, PerkinElmer makes no Warranty of any kind with regard to this document, including, but not limited to, the implied warranties of merchantability and fitness for a particular purpose.

PerkinElmer shall not be liable for incidental or consequential damages in connection with the furnishing or use of this document.

**COPY**

### Component List

Component / Specific Model	Serial #	Configuration Notes
PinAAcle 900F	PFBS2208081	Syngistix Ver 5.0.1.2029

### Parts Lists

Parts Included with the PM		
Part Number (if applicable)	Description	Quantity
B0501696	Fan Filters	1
N3160156	O-Ring Kits for Sampling Introduction (Stainless Steels Nebulizer)	N/A
N3160157	O-Ring Kits for Sampling Introduction (Plastic Nebulizer)	2
N9301714	Replacement Acetylene Filter Cartridge	2
TH001022	Replacement Air Filter Cartridge	1

Additional Reagents and Standards Required for PM				
Part Number (if applicable)	Description	Quality	Batch/Lot #	Expired Date (MM/YY)
N9300183	1000 mg/L Copper Standard	AR	26-B7CUY1	APR-2025

Additional Reagents and Standards Required for PM (Customer Support Solution)				
Part Number (if applicable)	Description	Quantity	Batch/Lot #	Expiration Date (MM/YY)
N/A	DI Water	250 mL	AR	AR
N/A	0.5% HNO <sub>3</sub>	250 mL	AR	AR

**COPY**

Additional Tools Required for PM			
Part Number (If applicable)	Description	Quantity	Serial #
N1013000	0.2A Neutral density filter	1	MG0-135
N1013002	1.0A Neutral density filter	1	MG2-258
03030997	System 2 EDL Driver	1	030309-97E
N3050605	As System 2 EDL	1	17986
N3050121	Cu Lumina HCL	1	000003793D12
N3050109	Ba Lumina HCL	1	041123-010120
N3050139	K Lumina HCL	1	0000037B8E1D
N3050152	Ni Lumina HCL	1	

## Procedure Checklist

Use (✓) to check off those steps in the checklist that have been completed.

### 1. General:

- ☒ Review the instrument performance with the customer and document any recent problems.
- ☒ Inspect the customer log book and make any appropriate PM entries.
- ☒ Perform general inspection of system for cleanliness.

### 2. PC Instrument Software:

- ☒ Instrument Software user files/databases archived, packed, and/or deleted as needed.

### 3. Mechanical:

- ☒ Inspect and clean all fans and filters. Replace filters if necessary
- ☒ Inspect all gas lines for leaks and/or wear. Replace if needed.
- ☒ Clean exterior of the instrument.
- ☒ Inspect the burner head, burner chamber, and nebulizer. Clean if needed as stated in the Hardware Guide.
- ☒ Check burner head dimensions with the feeler gauge as stated in the Hardware Guide in the Maintenance chapter section on cleaning the burner head and checking sloth width. Replace if out of specification
- ☒ Check the condition of the end cap, burner head, and nebulizer O-rings. Replace if necessary.
- ☒ Check the drain system for signs of wear. Replace worn or damaged parts.
- ☒ Visually check for proper flame conditions when igniting the Air-C2H2 and N2O-C2H2 flames (if applicable).

### 4. Electrical:

- ☒ Inspect PC boards. Clean if necessary.
- ☒ Carefully check all internal and external cable connections.
- ☒ Check instrument firmware revisions upgrade to current levels (if necessary)
- ☒ Run Diagnostics Test within the Advanced function of the Spectrometer page. Check the results in the service log folder in the Spectrometer BM Log Viewer.

### 5. Optics:

- ☒ Inspect and clean the sample compartment windows, if needed.
- ☒ Inspect optics. Clean or replace if necessary,

### 6. Gasses:

- ☒ Verify that the Gasses supplied to the instrument are within the pressure and purity specifications found in the PinAAcle 900 Series Pre-installation Checklist SDB.
- ☒ Verify that the acetylene filter and air filter element is dry. Replace if necessary.

**COPY**

**COPY**

## 7. Flame Interlock Check:

Description: Check to ensure that all safety interlocks are closed.

Parameter	Specification	Test Results	Pass/Fail
Flame Sensor	Air/C <sub>2</sub> H <sub>2</sub> Flame correctly shuts down	Active <input type="checkbox"/>	Passed <input type="checkbox"/>
Drain Sensor	Air/C <sub>2</sub> H <sub>2</sub> Flame correctly shuts down	Active <input type="checkbox"/>	Passed <input type="checkbox"/>
Nebulizer Sensor	Air/C <sub>2</sub> H <sub>2</sub> Flame correctly shuts down	Active <input type="checkbox"/>	Passed <input type="checkbox"/>
C <sub>2</sub> H <sub>2</sub> Pressure Sensor	Air/C <sub>2</sub> H <sub>2</sub> Flame correctly shuts down	Active <input type="checkbox"/>	Passed <input type="checkbox"/>
Air Pressure Sensor	Air/C <sub>2</sub> H <sub>2</sub> Flame correctly shuts down	Active <input type="checkbox"/>	Passed <input type="checkbox"/>
Burner Head Sensor	Choosing Nitrous Oxide as the oxidant should trigger an Interlock shuts down	Active <input type="checkbox"/>	Passed <input type="checkbox"/>

## 8. After PM Performance tests:

### 8.1 Detector Linearity with Barium

Description: Ensures that the detector is linear in the Visible Range.

Parameter	Specification	Certificate Value at 553.6 nm (Abs.)	Test Results	Pass/Fail
1.0 A ND Filter	± 5% from Cert.	0.9995	0.9994	Passed <input type="checkbox"/>
0.2 A ND Filter	± 5% from Cert.	0.1936	0.1874	Passed <input type="checkbox"/>

### 8.2 Baseline Noise at 1.0 Absorbance with Barium

Description: Ensures that a high absorbance will not produce excessive noise.

Parameter	Specification	Results	Pass/Fail
Standard Deviation	≤ 0.010	0.0015	Passed <input type="checkbox"/>

### 8.3 AA Baseline Noise with Copper

Description: Check baseline noise.

Parameter	Specification	Results	Pass/Fail
Standard Deviation	≤ 0.001	0.0001	Passed <input type="checkbox"/>

### 8.4 D<sub>2</sub> Background Compensation with Copper

Description: Verifies the instruments ability to compensate for Background absorption.

Parameter	Specification	Results	Pass/Fail
Standard Deviation	≤ 0.010	0.0013	Passed

### 8.5 AA-BG Baseline Noise with Copper

Description: Ensures that background correction does not produce excessive noise.

Parameter	Specification	Results	Pass/Fail
Standard Deviation	≤ 0.005	0.0001	Passed

### 8.6 AA-BG Baseline Noise with Arsenic

Description: Ensures that background correction does not produce excessive noise at a low wavelength.

Parameter	Specification	Results	Pass/Fail
Standard Deviation	≤ 0.005	0.0001	Passed

### 8.7 Flame Sensitivity

Description: Instrument Sensitivity checked against Copper standard.

Standard Copper Sensitivity	Specification	Results (Abs.)	Pass/Fail
5 mg/L Sensitivity SS Neb (if applicable)	> 0.250 Abs.	N/A	Passed
2 mg/L Sensitivity HS Neb (if applicable)	> 0.250 Abs.	0.3402	Passed

## 10. Review:

- ☒ Review with the customer PM work performed.
- ☒ Review with the customer routine maintenance procedures.
- ☒ Discuss recommended customer supplied materials to have on hand.
- ☒ Attach PM sticker.

COPY

COPY

### Additional Comments

Additional Comments Regarding the PM

### Review

*The preventive maintenance checks and if applicable performance tests for PinAAcle 900F have been completed.*

*This PinAAcle 900F Passes ☒ Fails ☐ the preventive maintenance.*

#### Review of Preventive Maintenance:

Authorized PerkinElmer Representative:

Rasit

Date:

22 APR 2025

(DD-MMM-YYYY)

Authorized Customer Representative:

621025564

Date:

22 APR 2025

(DD-MMM-YYYY)

**COPY**

## **BAROMETER**

**Serial No. : N/A[S41020124]**





# CALIBRATION LABORATORY Co.,LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230  
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



## CERTIFICATE OF CALIBRATION

### FOR

NOMENCLATURE : BAROMETER  
MANUFACTURER : BARIO  
MODEL / TYPE : N/A  
SERIAL NO. : N/A[S41020124]  
CLID. NO. : 212500828  
JOB CONTROL NO. : 250507051351  
CALIBRATION SERVICE : ☒ IN-LABORATORY ☐ ON-SITE

CUSTOMER : EASTERN THAI CONSULTING 1992 CO., LTD.  
683 MOO 11, SUKHAPIBARN 8 RD,  
NONGKHAM, SRIRACHA, CHONBURI 20230

DATE OF RECEIVED : 07 May 2025

DATE OF ISSUED : 09 May 2025

The report of calibration shall not be reproduced except in full without approval of the Calibration Laboratory Co., Ltd.

Calibrated By : Sittipong Pimdee  
Calibration Engineer

Approved By : Mongkol Yotsoontorn  
Authorized Signatory  
09 May 2025



This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to the International System of Units (SI)

Certificate No. Q25051351

F3-011-05/12-23



# CALIBRATION LABORATORY Co.,LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230  
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



## REPORT OF CALIBRATION

### FOR

NOMENCLATURE : BAROMETER  
MANUFACTURER : BARIO  
MODEL / TYPE : N/A  
SERIAL NO. : N/A[S41020124]  
DATE OF CALIBRATION : 08 May 2025

#### ENVIRONMENT CONDITIONS :

Temperature : (23 ± 2) °C

Relative Humidity : (55 ± 10) %RH

#### PROCEDURE USED :

This instrument was calibrated under procedure No. CLC-CPPP-08 according to DKD-R 6-1 as calibration guidelines.  
The calibration was performed by direct measurement with Reference Pressure Monitor which maintained by the Calibration Laboratory Co., Ltd.

#### REFERENCE STANDARD USED :

Reference Pressure Monitor, Fluke Model RPM3 S/N. 829.

#### TRACEABILITY :

The measurements are traceable to International System of Units (SI), through National Institute of Metrology (Thailand).  
Certificate No. MP-0245-24, Due Date 11 November 2025.

#### UNCERTAINTY :

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor of  $k = 2$ . It has been evaluated according to the "Calibration of Pressure Gauges (DKD-R 6-1)" which provides a level of confidence approximately 95%.

Certificate No. Q25051351

F3-011-05/12-23

page 2 of 3





# CALIBRATION LABORATORY CO., LTD.

2/10-11,14,55 Soi Prasert Manukil 29 Yaek 4, Prasert Manukil Rd., Ladphrao, Bangkok 10230  
Tel: 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail: sale@cal-laboratory.com



**CONDITION OF CALIBRATION ITEM : RECEIVED IN GOOD OPERATIONAL CONDITION**

**MEASUREMENT RESULTS : ( X ) without adjustment ( ) adjustment**

The DUC was exercised by applying a known pressure from its zero to full scale 1 times. Then 2 series of known gauge pressure were applied. The STD reading were recorded and the means value were reported in the table below.

## CALIBRATION DATA

### **CORRECTION OF PRESSURE**

DUC Test point ( hPa )	STD Reading ( hPa )		Correction ( hPa )	
	Up	Down	Up	Down
990	990.7	990.7	+0.7	+0.7
1000	1000.7	1000.8	+0.7	+0.8
1010	1010.8	1010.8	+0.8	+0.8
1020	1020.8	1020.9	+0.8	+0.9
1030	1030.9	1030.9	+0.9	+0.9

Uncertainty of measurement  $\pm 0.7$  hPa

Transmitting fluid : Air.

Note, The Scope of Accredited ANAB Certificate No. ACDM-2814 Version 015 Page 44 of 68

**This report is valid for the above stated instrument/s only.**

### End of Certificate ###

Certificate No. Q25051351

F3-011-05/12-23

**COPY**



@clccalibration



# **BOD INCUBATOR**

**Model : LABE 19/3**



Page 1 of 3

## CERTIFICATE OF CALIBRATION

Certificate No. : 24-089291

Sample Code : 24-35676-001

Customer : EASTERN THAI CONSULTING 1992 CO., LTD.  
683 Moo 11, Sukhapibarn 8 Rd., Nongkham, Sriracha,  
Chonburi 20230

Location of Calibration : EASTERN THAI CONSULTING 1992 CO., LTD.  
(Laboratory)

Equipment : Temperature controlled enclosures (Incubator)

Manufacturer : พัด เครื่องเย็น Model : N/A

Serial No. : S43020027 ID No. : LABE 19/3

Date of Receipt : 16 July 2024 Date of Calibration : 16 July 2024

## Condition of Calibration

1. Environment
- |                           |   |         |           |   |         |           |
|---------------------------|---|---------|-----------|---|---------|-----------|
| 1.1 Ambient temperature   | : | Maximum | 30.6 °C   | : | Minimum | 28.9 °C   |
| 1.2 Relative humidity     | : | Maximum | 76.9 %    | : | Minimum | 69.4 %    |
| 1.3 Line voltage supplied | : | Maximum | 219.8 VAC | : | Minimum | 217.1 VAC |

## 2. Calibration method

TLAS-G-20: Guidelines for calibration and checks of temperature controlled enclosures.

## 3. Reference standard instrument

Instrument	ID No.	Certificate No.	Due Date
Data acquisition with sensor (RTD-P1100)	LB-DA-12 (RTD-168 to RTD-176)	24-045389	28 April 2025

## 4. This certificate is traceable to the international system of unit (SI Unit).

The measurement is traceable to Asia Medical and Agricultural Laboratory and Research Center Public Company Limited.

## 5. This result of calibration was found accurate as shown on date and place of calibration only.

## 6. Condition of calibration item : Normal

Calibrated by Mr. Pattanapong Pulngern

Scientist

Approved by

(Mr. Somchai Neampunt)

Signed for Director

Issue date 17 July 2024

The uncertainties are for a confidence probability of approximately 95%.

The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only.

This Certificate is Issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Asia Medical and Agricultural Laboratory and Research Center Public Company Limited (AMARC)



Page 2 of 3

## REPORT OF CALIBRATION

Certificate No. : 24-089291

Sample Code : 24-35676-001

## Results of Calibration

Resolution : 0.1 °C

## 1. Reporting of Temperature

Calibration point (°C)	UUC* setting (°C)	UUC* reading (°C)	Measured temperature at each positions (°C)									Uncertainty ± (°C)	Coverage factor k
			# 1	# 2	# 3	# 4	# 5	# 6	# 7	# 8	# 9 <sup>Rev</sup>		
20	20.0	20.0	20.56	20.45	20.01	19.85	20.21	20.25	20.17	20.05	20.11	0.24	2.00

## 2. Characterization results

Calibration point (°C)	Stability ± (°C)	Uniformity (°C)	Overall variation (°C)
20	0.08	0.50	0.87

## Notes

- UUC\* = Unit Under Calibration

COPY

## REPORT OF CALIBRATION

Certificate No. : 24-089291

Sample Code : 24-35676-001

## Results of Calibration

## Notes

## 1. Sensor installation locations

1.1 All sensors at any corners or walls should be positioned

5 cm (a x b x c) from the wall.

1.2 The reference sensor is preferably located of the geometric center of the chamber.

## 2. Interior dimensions approx of chamber :

W = 70 cm ; D = 55 cm ; H = 140 cm

## 3. Air valve or fresh air level : Off

## 4. Fan level : Open

## 5. The quoted uncertainty includes "Stability of chamber and loading effect in chamber at 20% of uniformity".


## 6. Uniformity - the maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time.

## 7. Stability - one-half of the greatest maximum difference of measured temperatures at any one sensor.

## 8. Overall variation - the difference of the maximum and the minimum measured temperatures throughout observation time.

## 9. UUC\* reading - the average reading of indicating device that forms the integral part of the enclosure.

## 10. Calibration results without adjustment.

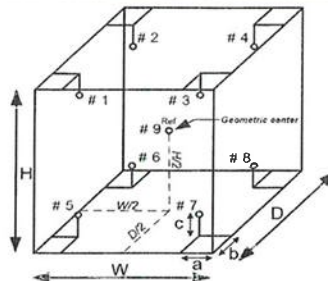Figure: Example of sensor  
installation Positions

The result expanded uncertainty of measurement  $U$  is stated as the standard uncertainty of measurement multiplied by the coverage factor  $k$ , which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty of measurement has been determined in accordance with UKAS M3003.

- End of Report -



# **BOD INCUBATOR**

**Model : LABE 19/5**



Page 1 of 3

## CERTIFICATE OF CALIBRATION

Certificate No. : 25-042561  
Sample Code : 25-18090-002Customer : EASTERN THAI CONSULTING 1992 CO., LTD.  
683 Moo 11, Sukhapibarn 8 Rd., Nongkham,  
Sriracha, Chonburi 20230Location of Calibration : EASTERN THAI CONSULTING 1992 CO., LTD.  
(Laboratory)

Equipment : Temperature controlled enclosures (Incubator)

Manufacturer : Lovibond Model : TC 445 S

Serial No. : 0520/005227 ID No. : LABE 19/5

Date of Receipt : 20 March 2025 Date of Calibration : 20 March 2025

## Condition of Calibration

1. Environment
- |                           |   |
|---------------------------|---|
| 1.1 Ambient temperature   | : Maximum 29.9 °C ; Minimum 27.5 °C     |
| 1.2 Relative humidity     | : Maximum 51.9 % ; Minimum 43.4 %       |
| 1.3 Line voltage supplied | : Maximum 239.4 VAC ; Minimum 232.8 VAC |

## 2. Calibration method

TLAS-G-20: Guidelines for calibration and checks of temperature controlled enclosures.

## 3. Reference standard instrument

Instrument	ID No.	Certificate No.	Due Date
Data Acquisition With Sensor (RTD-Pt100)	LB-DA-11 (RTD-148 to RTD-155, RTD-227)	24-040190	03 April 2025

## 4. This certificate is traceable to the international system of unit (SI Unit).

The measurement is traceable to Asia Medical and Agricultural Laboratory and Research Center Public Company Limited.

## 5. This result of calibration was found accurate as shown on date and place of calibration only.

## 6. Condition of calibration item : Normal

Calibrated by Mr. Pattanapong Pulngern

Scientist

Approved by

(Mr. Somchai Neampunt)

Signed for Director

Issue date 24 March 2025

The uncertainties are for a confidence probability of approximately 95%.

The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Asia Medical and Agricultural Laboratory and Research Center Public Company Limited (AMARC).



Page 2 of 3

## REPORT OF CALIBRATION

Certificate No. : 25-042561

Sample Code : 25-18090-002

## Results of Calibration

Resolution : 0.1 °C

## 1. Reporting of Temperature

Calibration point (°C)	UUC* setting (°C)	UUC* reading (°C)	Measured temperature at each positions (°C)									Uncertainty ± (°C)	Coverage factor k
			# 1	# 2	# 3	# 4	# 5	# 6	# 7	# 8	# 9 <sup>Ref</sup>		
20	20.5	20.5	19.91	19.78	19.82	19.86	19.78	19.85	19.93	19.63	19.79	0.38	2.00

## 2. Characterization results

Calibration point (°C)	Stability ± (°C)	Uniformity (°C)	Overall variation (°C)
20	0.28	0.25	0.83

## Notes

- UUC\* = Unit Under Calibration

NSC-TISI-TIS17025  
CALIBRATION 0152

Page 3 of 3

## REPORT OF CALIBRATION

Certificate No. : 25-042561

Sample Code : 25-18090-002

## Results of Calibration

## Notes

- Sensor installation locations
  - All sensors at any corners or walls should be positioned 5 cm (a x b x c) from the wall.
  - The reference sensor is preferably located of the geometric center of the chamber.
- Interior dimensions approx of chamber :  
W = 60 cm ; D = 56 cm ; H = 146 cm
- Air valve or fresh air level : Off
- Fan level : Open
- The quoted uncertainty includes "Stability of chamber and loading effect in chamber at 20% of uniformity %".
- Uniformity - the maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time.
- Stability - one-half of the greatest maximum difference of measured temperatures at any one sensor.
- Overall variation - the difference of the maximum and the minimum measured temperatures throughout observation time.
- UUC\* reading - the average reading of indicating device that forms the integral part of the enclosure.
- Calibration results without adjustment.

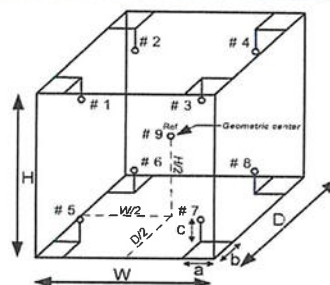


Figure: Example of sensor  
Installation Positions

The result expanded uncertainty of measurement  $U$  is stated as the standard uncertainty of measurement multiplied by the coverage factor  $k$ , which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty of measurement has been determined in accordance with UKAS M3003.

- End of Report -

**COPY**

**Hot Air Oven**

**Model : UM 400**

**Serial No. : 900982**





Page 1 of 3

## CERTIFICATE OF CALIBRATION

Certificate No. : 24-164692  
Sample Code : 24-67405-002

Customer : EASTERN THAI CONSULTING 1992 CO., LTD.  
683 Moo 11, Sukhapibarn 8 Rd, Nongkham,  
Sriracha, Chonburi 20230

Location of Calibration : EASTERN THAI CONSULTING 1992 CO., LTD.  
(Hot Lab)

Equipment : Temperature controlled enclosures (Hot air oven)

Manufacturer : Memmert Model : UM 400

Serial No. : 900982 ID No. : LABE 17/1

Date of Receipt : 19 December 2024 Date of Calibration : 19 December 2024

## Condition of Calibration

1. Environment
- |                           |   |
|---------------------------|---|
| 1.1 Ambient temperature   | : Maximum 32.1 °C ; Minimum 30.4 °C     |
| 1.2 Relative humidity     | : Maximum 48.9 % ; Minimum 42.4 %       |
| 1.3 Line voltage supplied | : Maximum 226.3 VAC ; Minimum 221.0 VAC |

## 2. Calibration method

TLAS-G-20: Guidelines for calibration and checks of temperature controlled enclosures.

## 3. Reference standard instrument

Instrument	ID No.	Certificate No.	Due Date
Data Acquisition With Sensor (RTD-Pt100)	LB-DA-11 (RTD-148 to RTD-155, RTD-227)	24-040190	03 April 2025

## 4. This certificate is traceable to the international system of unit (SI Unit).

The measurement is traceable to Asia Medical and Agricultural Laboratory and Research Center Public Company Limited.

## 5. This result of calibration was found accurate as shown on date and place of calibration only.

## 6. Condition of calibration item : Normal

Calibrated by Mr. Nophanon Anusak  
Scientist

Approved by

(Mr. Somchai Neampunt)  
Signed for Director

Issue date 20 December 2024

The uncertainties are for a confidence probability of approximately 95%.

The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Asia Medical and Agricultural Laboratory and Research Center Public Company Limited (AMARC).



Page 2 of 3

## REPORT OF CALIBRATION

Certificate No. : 24-164692  
Sample Code : 24-67405-002

## Results of Calibration

Resolution : 0.1 °C

## 1. Reporting of Temperature

Calibration point (°C)	UUC* setting (°C)	UUC* reading (°C)	Measured temperature at each positions (°C)									Uncertainty ± (°C)	Coverage
			# 1	# 2	# 3	# 4	# 5	# 6	# 7	# 8	# 9 <sup>Ref</sup>		factor k
85	85.0	85.0	85.33	85.28	84.83	85.01	85.15	85.18	85.32	85.12	85.23	0.25	2.00

## 2. Characterization results

Calibration point (°C)	Stability ± (°C)	Uniformity (°C)	Overall variation (°C)
85	0.10	0.43	0.69

## Notes

- UUC\* = Unit Under Calibration

**COPY**

## REPORT OF CALIBRATION

Certificate No. : 24-164692

Sample Code : 24-67405-002

## Results of Calibration

## Notes

1. Sensor installation locations
  - 1.1 All sensors at any corners or walls should be positioned 5 cm ( $a \times b \times c$ ) from the wall.
  - 1.2 The reference sensor is preferably located of the geometric center of the chamber.
2. Interior dimensions approx of chamber :  
W = 40 cm ; D = 28 cm ; H = 39 cm
3. Air valve or fresh air level : Off
4. Fan level : Open
5. The quoted uncertainty includes " Stability of chamber and loading effect in chamber at 20% of uniformity ".
6. Uniformity - the maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time.
7. Stability - one-half of the greatest maximum difference of measured temperatures at any one sensor.
8. Overall variation - the difference of the maximum and the minimum measured temperatures throughout observation time.
9. UUC\* reading - the average reading of indicating device that forms the integral part of the enclosure.
10. Calibration results without adjustment.

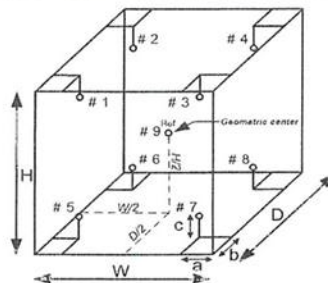


Figure: Example of sensor  
installation Positions

The result expanded uncertainty of measurement  $U$  is stated as the standard uncertainty of measurement multiplied by the coverage factor  $k$ , which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty of measurement has been determined in accordance with UKAS M3003

- End of Report -


**COPY**

**ICP-OES/Avio550**

**Serial No. : M81S221010**

### ICP-OES/Avio500 Preventive Maintenance (PM)

<b>Company Name:</b>	Eastern Thai Consulting 1992 Co.,Ltd		
<b>Address (Instrument Location):</b>	683 Moo 11, Nong Kham Subdistrict, Si Racha District, Chonburi		
<b>Serial Number:</b>	M81S221010	<b>PM Number:</b>	1 of 2
<b>Customer Name (if applicable):</b>	Channarong	<b>Telephone Number:</b>	0968761232
<b>Service Engineer Name:</b>	Khwanchai	<b>Service Order Number:</b>	WO-03149107
<b>Date PM Performed: (DD-MMM-YYYY)</b>	22-Apr-2025	<b>Next PM Due Date: (DD-MMM-YYYY)</b>	22-Oct-2025
<b>Standard Labor Hours to Complete PM :</b>		<b>4 hours</b>	

Part Number	Release	Publication Date	
TH09370188 Rev.1	B	July 2020	

#### Scope

The purpose of this PM is to ensure the continued functionality of the PerkinElmer / Avio500 by inspecting and replacing any worn or damaged parts. This service should only be performed by a trained representative of PerkinElmer. The customer should save their method before the PM begins.

#### General Instructions:

The customer must provide the engineer operational data to demonstrate recent instrument performance prior to starting the PM.

Always check with the customer before making any changes that may affect the customer's analysis or calibration, including a current back-up of system software and/or data files. The completed document should be signed by an authorized PerkinElmer and customer representative and left with the customer. Update the PM sticker and instrument logbook as required.

#### Copyright Information

This document contains proprietary information that is protected by copyright. All rights are reserved. No part of this publication may be reproduced in any form whatsoever or translated into any language without the prior, written permission of PerkinElmer, Inc. Copyright © 2013 PerkinElmer, Inc.

#### Trademarks

Registered names, trademarks, etc. used in this document, even when not specifically marked as such, are protected by law. PerkinElmer is a registered trademark of PerkinElmer, Inc. All other trademarks and registered trademarks not owned by PerkinElmer, Inc. or its subsidiaries that are depicted herein are the property of their respective owners.

Except as specifically set forth in its terms and conditions of sale, PerkinElmer makes no Warranty of any kind with regard to this document, including, but not limited to, the implied warranties of merchantability and fitness for a particular purpose.

PerkinElmer shall not be liable for incidental or consequential damages in connection with the furnishing or use of this document.

### Component List

Component / Specific Model	Serial #	Configuration Notes

### Parts Lists

Parts Included with the PM		
Part Number (if applicable)	Description	Quantity
09995098	Air Filter-Spectrometer	1
N077520	Air Filter-RF Generator	1
09992731	Axial Window	1
B0810377	Radial Window	1
N0770438	O-ring kit, injector support adapter	1
N0780437	O-ring kit, torch	1

Additional Reagents and Standards Required for PM				
Part Number (if applicable)	Description	Quality	Batch/Lot #	Expired Date (MM/YY)
N0691579	Muti-Element Standard	AR	62-162CRX1	Dec-25
N9300221	DL Standard diluted 100 X	AR	61-190CRY1	Aug-25
N0582152	Wave Cal Solution	AR	63-059CRX1	Oct-25
N9302946	VIS Wavecal Solution	AR	61-167CRT1	Dec-25

**COPY**

## Procedure Checklist

Use (✓) to check off those steps in the checklist that have been completed.

### 1. General:

- ☒ Ask customer about unit's performance since last visit.
- ☒ Check incoming AC line voltage under load for proper levels and grounding.
- ☒ Is the instrument operational? If not, please comment.

### 2. Mechanical:

- ☒ Inspect and clean all fans and filters.
- ☒ Inspect and replace torch components and necessary.

Torch Components Replaced: ☒ Yes ☐ No

- ☒ Inspect all tubing for signs of cracking or leaking and replace as necessary.

Tubing Replaced: ☐ Yes ☒ No

- ☒ Inspect the peristaltic pump for proper operation.
- ☒ Check and adjust if necessary, the external nitrogen, argon shear gas and water supply pressures.
- ☒ Check and adjust if necessary, the internal nitrogen, main argon, torch argon and shear gas pressures.

Regulator	Measured Pressure	Set Pressure
Nitrogen		NA (calibrated In Factory)
Main Argon	76	76 psig
Torch Argon	67	67 psig
Shear Gas	65	65 psig
Water	35	35 psig

- ☒ Check shear gas nozzle for blockages and proper, uniform flow.
- ☒ Inspect nitrogen Hi/Low purge and shear gas solenoids for proper function.
  - ☒ Inspect the function of all spectrometer motors. Drive the motors from the Spectrometer DCM. (slits, XY motor)
- ☒ Inspect the function of the pneumatic shutter for proper operation.
  - ☒ Perform preventative maintenance on the chiller as required. Make the customer aware of the importance of maintaining the chiller fluid level and filter replacement.
- ☒ Drain air compressor surge tank.
- ☒ Clean exterior of instrument.
- ☒ Visually inspect all PC boards for cleanliness and signs of corrosion.

**COPY**

### 3. Electrical

- ☒ Check all RF generator and spectrometer power supply voltages.
- ☒ Run instrument diagnostic checks from the appropriate Device Control Module.

#### RF Generator:

- ☒ Check the RF generator status screens.
- ☒ Check the function of all interlocks.

#### Spectrometer:

- ☒ Check the spectrometer status screens. Ensure Ready mode with no fatal errors.
- ☒ Check the spectrometer optical tub temperatures (top, bottom, fin, optical base).
- ☒ Check detector temperatures.
- ☒ Check TEC voltages (6.5VDC)

### 4. Optical:

- ☒ Clean or replace the axial and radial view windows as necessary.
  - Axial Window Replaced: ☒ Yes ☐ No
  - Radial Window Replaced: ☒ Yes ☐ No

### 5. PM Performance Tests:

- ☒ Perform View Align.

#### Test Spectral Resolution:

- ☒ Measure the spectrometers ability to separate two adjacent wavelengths.

Parameter	Specification	Test Result	Pass/Fail
As 193.696 - Resolution	≤0.007	0.00530	Passed
Ni 231.604 - Resolution	≤0.008	0.00730	Passed
Ni 341.476 - Resolution	≤0.012	0.00893	Passed
La 408.672 - Resolution	≤0.020	0.01603	Passed
Ba 455.403 - Resolution	≤0.025	0.02038	Passed

#### Test Precision:

- ☒ Test for reproducibility of a set of measurement.

Parameter	Specification	Test Result	Pass/Fail
As 193.696	%RSD ≤ 1 %	0.32	Passed
Zn 213.856	%RSD ≤ 1 %	0.18	Passed
Mn 257.610	%RSD ≤ 1 %	0.21	Passed
La 379.478	%RSD ≤ 1 %	0.13	Passed
Ba 455.403	%RSD ≤ 1 %	0.15	Passed
Ba 493.408	%RSD ≤ 1 %	0.20	Passed

**COPY**



☒ Run an Axial & Radial BEC according to the A&T spec.

**Test Axial BEC Cd:**

Method "BEC-XL" For Samples "IB (2%HNO3)" and "IS (N930-0221/100)", record intensities.

Calculated BEC:  $BEC = (IB * Conc\ of\ Std) / (IS - IB)$ . Where Conc of Std = 500 PPB

Element	Conc.	IB	IS	
Cd 226	500	1199.8	209735	
IB*Conc	IS-IB	BEC	Spec	Pass/Fail
599900	208535.2	2.88	<150 PPB	Passed

**Test Radial BEC Mn:**

Method "BEC-RL" For Samples "IB (2%HNO3)" and "IS (N069-1579)", record intensities.

Calculated BEC:  $BEC = (IB * Conc\ of\ Std) / (IS - IB)$ . Where Conc of Std = 1,000 PPB

Element	Conc.	IB	IS	
Mn 257	1,000	653.2	217211.6	
IB*Conc	IS-IB	BEC	Spec	Pass/Fail
653200	216558.4	3.02	<45 PPB	Passed

**6. Review:**

- ☒ Review with the customer PM work performed.
- ☒ Discuss recommended customer supplied materials to have on hand.
- ☒ Attach PM sticker.

## Additional Comments

### Additional Comments Regarding the PM

- Use with Sample introduction AQ for PM test

## Review

*The preventive maintenance checks and if applicable performance tests for ICP-OES/Avio500 have been completed.*

*This ICP-OES/Avio500 Passes ☒ Fails ☐ the preventive maintenance.*

### Review of Preventive Maintenance:

Authorized PerkinElmer Representative:	<i>KLS</i>	Date: 22-Apr-2025 (DD-MMM-YYYY)
Authorized Customer Representative:		Date: 22-Apr-2025 (DD-MMM-YYYY)

**LIQUID IN GLASS THERMOMETER**

**Model / Type : 0-100 °C**

**Serial No. : 43560**





# CALIBRATION LABORATORY Co., LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230  
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



## CERTIFICATE OF CALIBRATION

### FOR

NOMENCLATURE : LIQUID IN GLASS THERMOMETER  
MANUFACTURER : AA PRECISION  
MODEL / TYPE : 0-100 °C  
SERIAL NO. : 43560[LABE 16/1]  
CLID. NO. : 232403905  
JOB CONTROL NO. : 241031116258  
CALIBRATION SERVICE : ☒ IN-LABORATORY ☐ ON-SITE

CUSTOMER : EASTERN THAI CONSULTING 1992 CO., LTD.  
683 MOO 11, SUKHAPIBARN 8 RD,  
NONGKHAM, SRIRACHA, CHONBURI 20230

DATE OF RECEIVED : 31 October 2024

DATE OF ISSUED : 05 November 2024

The report of calibration shall not be reproduced except in full without approval of the Calibration Laboratory Co., Ltd.

Calibrated By : Pimsiri Hemtanon  
Calibration Engineer

Approved By : Mongkol Yotsoontorn  
Authorized Signatory  
05 November 2024



This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to the International System of Units (SI)

COPY

Certificate No. Q24116258

F3-011-05/12-23

page 1 of 3



@clccalibration



# CALIBRATION LABORATORY Co., LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230  
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



## REPORT OF CALIBRATION

### FOR

NOMENCLATURE : LIQUID IN GLASS THERMOMETER  
MANUFACTURER : AA PRECISION  
MODEL / TYPE : 0-100 °C  
SERIAL NO. : 43560[LABE 16/1]  
DATE OF CALIBRATION : 04 November 2024

#### ENVIRONMENT CONDITIONS :

Temperature :  $(23 \pm 2) ^\circ\text{C}$

Relative Humidity :  $(55 \pm 10) \% \text{ RH}$

#### PROCEDURE USED :

This instrument was calibrated under procedure No. CLC-CPH-02 based on ASTM E 77-07 as calibration guidelines.  
The calibration was performed by comparison with Calibration Bath, Precision Thermometer and IPT  
which maintained by the Calibration Laboratory Co., Ltd.

#### REFERENCE STANDARD USED :

1. Calibration Bath, Kambic Model OB-22/2 ULT,OB-22/2 S/N. 17115653,17115654.
2. Precision Thermometer, ASL Model F200-A-8 S/N. 014433/03 with IPT S/N. L0193A-1-1,PO106346-1-18.

#### TRACEABILITY :

1. The measurements are traceable to International System of Units (SI), through Calibration Laboratory Co., Ltd. Certificate No. Q23136342,Q23126517. Due Date 20 December 2024,20 November 2024.
2. The measurements are traceable to International System of Units (SI), through Thailand Institute of Scientific and Technological Research (TISTR) and National Institute of Metrology (Thailand). Certificate No. PSL-T 0203/67,TT-0136-23,TT-0110-24. Due Date 07 December 2024,12 December 2024,06 August 2025.

#### UNCERTAINTY :

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor  $k = 2,00$  which for a normal distribution corresponds to a coverage probability of approximately 95 %.  
It has been evaluated according to the "Evaluation of the Uncertainty of Measurement in Calibration (EA-4/02 M:2022)"

Certificate No. Q24116258

F3-011-05/12-23

COPY

page 2 of 3



@clccalibration



# CALIBRATION LABORATORY Co., LTD.

2/10-11,14,55 Soi Prasert Manukil 29 Yaek 4, Prasert Manukil Rd., Ladphrao, Bangkok 10230  
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail sale@cal-laboratory.com



**CONDITION OF CALIBRATION ITEM : RECEIVED IN GOOD OPERATIONAL CONDITION**

**MEASUREMENT RESULTS : ( X ) without adjustment ( ) adjustment**

The DUC Reading were recorded and the means value were reported of four times measurement in the table below.

## CALIBRATION DATA

### **CORRECTION OF TEMPERATURE**

STD Reading ( °C )	DUC Reading ( °C )	Correction ( °C )	Uncertainty $\pm$ ( °C )
0.039	0.00	+0.039	0.065
25.003	25.00	+0.003	
50.008	50.00	+0.008	
100.013	100.00	+0.013	

Range : 0 °C to 100 °C

Graduation : 0.1 °C

Immersion Type : Total Immersion.

Correction of Reference Temperature ( 0 °C ) = 0.039 °C

Note. The Scope of Accredited ANAB Certificate No. ACDM-2814 Version 012 Page 56 of 67

**This report is valid for the above stated instrument/s only.**

### End of Certificate ###

Certificate No. Q24116258

F3-011-05/12-23

**COPY**

page 3 of 3



@dcalibration

**MERCURY ANALYZER**

**Model : RA-4500**

**Serial No. : 21780504**

Eastern Thai Consulting 1992

## Automatic Mercury Analyzer

Model : RA-4500

### Preventive Maintenance Report

SERIAL No. RA-4500 : 21780504

Soft version : Ver 2.0.8

ROM version : Ver 2.0.2

DATE : 3 FEBRUARY 2025

DUE DATE : 3 AUGUST 2025

INSPECTED BY : *Chayanant T.*  
( Chayanant T. )

APPROVED BY : *Natthaphong P.*  
( Natthaphong P. )



**Kinetic Solutions Company Limited.**

2, Soi Lat Krabang 1, Lat Krabang Subdistrict,

Lat Krabang District, Bangkok 10520

Tel. (+66) 062-789-5221

บริษัท ไคเนติก โซลูชั่น จำกัด  
KINETIC SOLUTIONS CO., LTD.

**COPY**

## Inspection

ITEMS	SPECIFICATIONS	RESULT	JUDGE
1. Quantity	-	Accessories are completed.	GOOD OK
2. Appearance	2.1 Overall Appearance	No visible damage.	GOOD OK
	2.2 Parts / Cables	Correctly placed and connected.	
3. Indication	Nameplate / Label	Plate and Label are indicated.	GOOD OK
4. Self check			
4.1 GLP Counter	Mercury Lamp	5000 hours	1625 hr OK
	Membrane Filter	2000 hours or 1 year after replace	830 hr OK
	Main Pump Tube	750 hours or 1 year after replace	721 hr OK
	Absorbed Hg	1500 mg	2 mg OK
	P1 Tube	2000 hours or 1 year after replace	109 hr OK
	P2 Tube	2000 hours or 1 year after replace	12 hr OK
	P3 Tube	2000 hours or 1 year after replace	11 hr OK
	P4 Tube	2000 hours or 1 year after replace	96 hr OK
	P5 Tube	2000 hours or 1 year after replace	10 hr OK
	P6 Tube	2000 hours or 1 year after replace	28 hr OK
	P7 Tube	2000 hours or 1 year after replace	27 hr OK
	Heater	2000 hours	1254 hr OK
4.2 Check/Test	Flow rate Adjustment	Flow rate 0.14 - 0.20 L/min	0.19 L/min OK
	Signals Detector	V.SIG is 3.5 - 4.5 V.	3.50 V. OK
		V.REF is 3.5 - 4.5 V.	3.52 V. OK
	Cooling Fan	Check the operation of cooling fan	PASS OK
	Color Sensor	signals (R,G,B) at least one nonzero	PASS OK
	Radiation Thermometer	a positive valve form thermometer	PASS OK
	Heater	heater temp rises 4 °C within 5 min.	PASS OK
5. Heater	Temperature	At 95°C ± 2°C with 30 min.	94.7°C OK
6. Calibration Curve	no pretreatment	0-100 ng : Max.Dev. ≤ 5.0%	3.40% OK
7. Repeatability	50 ug/L, 500ul, 25ng (n=5)	Average: 50ug/L ± 0.05 ug/L	51.06412 ug/L OK
		C.V. ≤ 5.0%	0.87% OK
8. Blank	no pretreatment	Less than 0.02 (AREA)	0.0025 AREA OK

### Apparatus

NAME	Date Certified	Expiration
Mercury ICP Standard (1000 ug/mL) AccuStandard, Inc. Lot 223035027	March 10, 2023	March 10, 2028

### Inspection details

**COPY**

## Inspection details

### Remark

#### 1. Cleaning Mercury Analyzer RA-4500

- Body case, Reagent Tube, Cell Detector, Table of Sample, Measurement Probe, Rinse Tube


#### 2. Checking Mercury Analyzer RA-4500

- Mercury Lamp
- Membrane Filter
- Main Pump Tube
- Motor Pump
- Motor Reagent pump
- Motor of Arm
- Motor of Table
- Motor of Lift
- Outlet Activated Carbon Filter
- Flow Sensor
- Valves
- Heater
- Cooling Fan
- Instrument Performance

#### 3. Inspection Calibration curve and Reproducibility of Mercury Analyzer RA-4500


Title : Preventive Maintenance Mercury Analyzer RA-4500 SN21780504  
 Date : 03-Feb-25  
 Name : Kinetic solutions  
 Memo : Calibration Curve 0 - 100 ng

Calib



### STD

No.	STD [ppm]	SVOL [mL]	CVOL [mL]	DVOL [mL]	STD [ng]	AREA [ON]	MEAS [ng]	Dev [%]	Note
1	0.000	0.000	5.000	5.000	0.000	0.0157	-0.0679	-	
2	0.050	0.100	5.000	5.000	5.000	6.0656	4.8276	3.4	
3	0.050	0.200	5.000	5.000	10.000	12.3481	9.9113	0.9	
4	0.050	0.500	5.000	5.000	25.000	31.2619	25.2160	0.9	
5	1.000	0.050	5.000	5.000	50.000	62.2600	50.2991	0.6	
6	1.000	0.100	5.000	5.000	100.000	123.4511	99.8139	0.2	

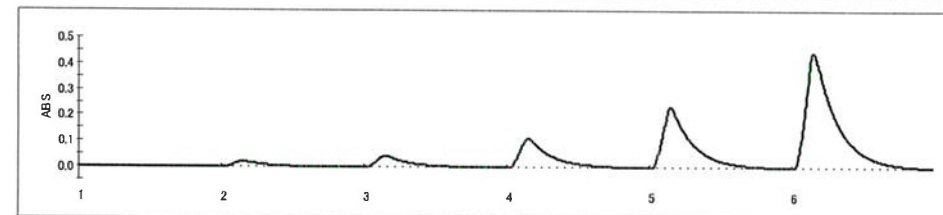

### SMP


No.	NAME	SVOL [mL]	CVOL [mL]	DVOL [mL]	AREA [ON]	MEAS [ng]	CONC [ug/L]	Note
1	50ppb, 500ul, 25ng	0.500	5.000	5.000	31.4230	25.3464	50.6928	
2	50ppb, 500ul, 25ng	0.500	5.000	5.000	31.3033	25.2495	50.4990	
3	50ppb, 500ul, 25ng	0.500	5.000	5.000	31.9460	25.7696	51.5392	
4	50ppb, 500ul, 25ng	0.500	5.000	5.000	31.7697	25.6269	51.2538	
5	50ppb, 500ul, 25ng	0.500	5.000	5.000	31.8204	25.6679	51.3358	

### Statistics

No.	NAME	TRY	AV [ug/L]	SD [ug/L]	Cv [%]
1	50ppb, 500ul, 25ng	5	51.06412	0.4451766	0.87

COPY

COPY

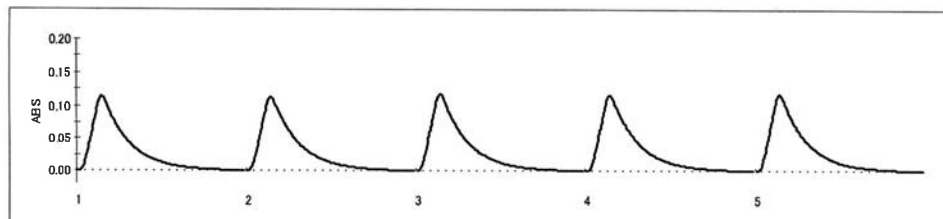


## Self Check

Heat check:PASS!! ( 24.9degC[05:00] -> 28.9degC[02:55])  
 Sensor check:PASS!! (1091- 69=1022)  
 Leak check:PASS!! (0.19L/min)  
 Sig/Ref check:PASS!! (Sig:3.50V, Ref:3.52V)  
 Drift check:PASS!! (-0.0054498 - -0.0059411 = 0.0004914)

Title : Preventive Maintenance Mercury Analyzer RA-4500 SN21780504  
 Date : 03-Feb-25  
 Name : Kinetic solutions  
 Memo : Blank

## SMP

No.	NAME	SVOL [mL]	CVOL [mL]	DVOL [mL]	AREA [ON]	MEAS [ng]	CONC [ug/L]	Note
1	blank	0.000	5.000	5.000	0.0025	-0.0786	0.0000	

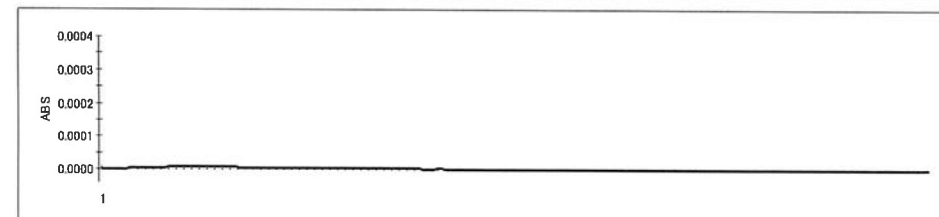

COPY

COPY





AccuStandard, Inc.

Tel (203) 786-5290  
Fax (203) 786-5287  
www.AccuStandard.com

# CERTIFICATE OF ANALYSIS

## AccuTrace™ Reference Standard

Catalog No: ICP-34N-1  
Description: Mercury ICP Standard  
Element: Mercury (Hg)  
SRM: 3133  
Lot: 223035027  
Matrix: 10% Nitric acid  
Hazards: Refer to SDS for complete safety information

Date Certified: Mar 10, 2023  
Expiration: Mar 10, 2028  
Density: 1.052 g/mL  
Sample Size: 100 mL  
Components: 1  
Storage Condition: Ambient (>5 °C)

### Certified Reference Material



### Certified Concentration: 1000 µg/mL

#### Trace Elements in µg/mL

Ag nd<0.02	Ce nd<0.2	Gd nd<0.02	Lu nd<0.02	Pb nd<0.2	Sc nd<0.02	Ti nd<0.02
Al nd<0.02	Co nd<0.02	Ge nd<0.2	Mg nd<0.02	Pd nd<0.2	Se nd<0.2	Tl nd<0.2
As nd<0.2	Cr nd<0.02	Hf nd<0.02	Mn nd<0.02	Pr nd<0.2	Si N/A	Tm nd<0.02
Au nd<0.02	Cs N/A	Hg *	Mo nd<0.02	Pt nd<0.2	Sm nd<0.2	U nd<0.2
B nd<0.2	Cu nd<0.02	Ho nd<0.02	Na nd<0.02	Rb N/A	Sn nd<0.02	V nd<0.02
Ba nd<0.02	Dy nd<0.02	In nd<0.2	Nb nd<0.2	Re nd<0.2	Sr nd<0.02	W nd<0.2
Be nd<0.02	Er nd<0.02	Ir nd<0.2	Nd nd<0.02	Rh nd<0.2	Ta nd<0.2	Y nd<0.02
Bi nd<0.2	Eu nd<0.02	K nd<0.2	Ni nd<0.02	Ru nd<0.02	Tb nd<0.02	Yb nd<0.02
Ca nd<0.02	Fe nd<0.02	La nd<0.02	Os N/A	S N/A	Te nd<0.2	Zn nd<0.02
Cd nd<0.02	Ga nd<0.02	Li nd<0.02	P N/A	Sb nd<0.2	Th nd<0.02	Zr nd<0.02

This Certified Reference Material was verified in accordance with ISO/IEC 17025 (AT-1339) and ISO 17034 (AR-1463)

This solution was assayed gravimetrically, using a balance calibrated against weight sets, ID #88270, traceable to NIST

A product with a suffix (-1A, -2B, etc. or -01, -02, etc.) on its lot number has had its expiration date extended and is identical to the same lot number without the suffix.

This product contains mercury and MUST be disposed of in accordance with all federal, state and local regulations.

The gravimetric uncertainty for this product is ±0.24%. The CRM uncertainty is ±2.4%.

In order to verify the concentration(s), the final solution was checked by plasma emission spectroscopy (ICP) against material traceable to the above listed NIST SRM(s).

We use the highest purity raw materials available to minimize impurity levels in the final solution. Typically 99.999%+ pure starting materials are used as well as high purity acids and ASTM Type I 18 megohm deionized water.

All trace level elemental impurities were determined via plasma emission spectroscopy on the concentrate.

All weights are traceable through NIST, Test No. 684/291344-18 & 684/292805-19

All glassware used in preparation is Class A.

All bottles are acid leached and triple rinsed with deionized water prior to use.

Shake bottle prior to use and do not pipette directly out of the bottle. Use only cleaned Class A volumetric glassware. Keep bottle tightly capped.

Certified By:   
Megan O'Leary, Inorganic QA Manager

For use in routine laboratory analysis.

### 1. Quality Standards:

ISO 17034:2016 – General Requirements for the Competence of Reference Material Producers

ISO/IEC 17025:2017 – General Requirements for the Competence of Testing And Calibration Laboratories

ISO 9001:2015 – Quality Management System – Requirements  
Eagle Registrations

2. **Intended Use:** The product covered by this certificate is designed for calibration or for use in quality control procedures for the specified chemical compounds listed on the reverse side. This product can be used for quantification and/or identification. This product can also be used as a reference material to validate analytical procedures, subject to the conditions under Section 7.

3. **Manufacturing:** All balances are calibrated daily using an in-house procedure with weights that are compared annually to master weights and traceable to NIST. The balances are also calibrated annually by an ISO/IEC 17025 accredited calibration laboratory. Please refer to the NIST test number listed on the front of this certificate. Class A glassware is used in the manufacture and quality control of all standards. Good Laboratory Practices have been used throughout the preparation of this Standard.

4. **Homogeneity:** This product is sufficiently homogeneous and any sample size would be within the uncertainty budget.

5. **Stability:** The manufacturer guarantees the stability of this solution through the expiration date stated on the label, when handled and stored according to the conditions stated on the label.

6. **Uncertainty:** The uncertainty values as stated on the face of this certificate have been determined using the EURACHEM/CITAC Guide. We report a combined expanded uncertainty equal to the positive square root of the total variance of the uncertainty of the components using the following formula:  $u_c = \sqrt{(u(V))^2 + (u(m))^2 + (u(I))^2 + (u(R))^2}$ . This formula represents uncertainty components from the mass, volume, short-term stability, long-term stability and homogeneity factors associated with the production of this product. The expanded uncertainty, assumes a normal distribution and a coverage factor of  $k=2$  is chosen using approximately a 95% confidence level.

7. **Legal Notice and Limit of Liability:** This product is for routine laboratory analysis and research purposes only. The company's liability will be limited to replacement of product or refund of purchase price. Notice of claims must be made within thirty (30) days from date of delivery.

COPY



**pH Meter**

**Model : SevenCompact S220**

**Serial No. : B835349235**

Certificate Number CCP-0403-25

**Calibration Certificate**  
**SevenCompact™ pH/Ion Meter S220****Customer**

Company EASTERN THAI CONSULTING 1992 CO., LTD.

Address 683 Moo 11, Sukhaphiban 8 Rd., Nong Kham

Siracha

CHONBURI 20230

Customer ID number 301608441

Customer representative คุณ ศิริกร นาคฉันท

**Instrument**

Type SevenCompact™ S220

Instrument Serial Number B835349235

Internal identification LABE 11/6

Firmware version 1.20.06

**Technical specifications**

Measuring Range -1999.9 ... 1999.9 mV -2.000 ... 20.000 pH

Resolution 0.1 mV 0.001 pH

Limit of Error  $\pm 0.2$  mV  $\pm 0.002$  pH

Temperature range MTC -30.0 ... 130.0 °C

Temperature range ATC -5.0 ... 130.0 °C

Resolution 0.1 °C

Limit of Error  $\pm 0.1$  °C**Procedure Statement**

METTLER TOLEDO Certification SOP (Doc. No. ME-30027577B) will be used as referring documentation to adjust and certify the instrument indicated in the "Type" and "Serial number" section. The measurement results of this certification were obtained at ambient conditions.

COPY

Certificate Number CCP-0403-25

**Certification Tools****Certified digital voltmeter**

Manufacturer KEYSIGHT TECHNOLOGIES

Type 34461A

Control No. ANA143

Serial number MY60036967

Certificate number E1U2401054

Due date March 10, 2025

**Certified Temperature Resistors**

Manufacturer METTLER-TOLEDO

Type 51302410

Control No. ANA114

Serial number A275

Certificate number 73757

Due date February 12, 2026

Designation	Nominal value	Certified value
NTC 30 k $\Omega$ , 0 °C	94.980 k $\Omega$	94.9730 k $\Omega$
NTC 30 k $\Omega$ , 25 °C	30.000 k $\Omega$	29.9950 k $\Omega$
NTC 30 k $\Omega$ , 50 °C	10.969 k $\Omega$	10.9704 k $\Omega$
NTC 30 k $\Omega$ , 75 °C	4.528 k $\Omega$	4.5275 k $\Omega$
NTC 30 k $\Omega$ , 100 °C	2.070 k $\Omega$	2.0714 k $\Omega$
PT1000, 0 °C	1.000 k $\Omega$	1.0001 k $\Omega$
PT1000, 25 °C	1.0974 k $\Omega$	1.0975 k $\Omega$
PT1000, 50 °C	1.1940 k $\Omega$	1.1942 k $\Omega$
PT1000, 75 °C	1.2899 k $\Omega$	1.2900 k $\Omega$
PT1000, 100 °C	1.3851 k $\Omega$	1.3851 k $\Omega$

COPY

# METTLER TOLEDO

Certificate Number **CCP-0403-25**

## Certification Measurements

Designation	Certified value	Measured value	Max. Tolerance	Passed / Failed
-1900 mV	-1900.0 mV	-1899.98 mV	0.2 mV	Passed
-1000 mV	-1000.0 mV	-1000.00 mV	0.2 mV	Passed
-500 mV	-500.0 mV	-499.98 mV	0.2 mV	Passed
-180 mV	-180.0 mV	-180.00 mV	0.2 mV	Passed
0 mV	0.0 mV	0.01 mV	0.2 mV	Passed
180 mV	180.0 mV	179.98 mV	0.2 mV	Passed
500 mV	500.0 mV	499.90 mV	0.2 mV	Passed
1000 mV	1000.0 mV	1000.00 mV	0.2 mV	Passed
1900 mV	1900.0 mV	1899.99 mV	0.2 mV	Passed

Designation	Measured low imp.	Measured high imp.	Max. Tolerance	Passed / Failed
1900 mV	1900.0 mV	1899.8 mV	0.6 mV	Passed

Designation	Nominal value	Measured value	Max. Tolerance	Passed / Failed
NTC 30 kΩ, 0 °C	0.0 °C	0.0 °C	0.1 °C	Passed
NTC 30 kΩ, 25 °C	25.0 °C	25.0 °C	0.1 °C	Passed
NTC 30 kΩ, 50 °C	50.0 °C	50.0 °C	0.1 °C	Passed
NTC 30 kΩ, 75 °C	75.0 °C	74.9 °C	0.1 °C	Passed
NTC 30 kΩ, 100 °C	100.0 °C	100.0 °C	0.1 °C	Passed
PT1000, 0 °C	0.0 °C	0.1 °C	0.1 °C	Passed
PT1000, 25 °C	25.0 °C	25.0 °C	0.1 °C	Passed
PT1000, 50 °C	50.0 °C	50.0 °C	0.1 °C	Passed
PT1000, 75 °C	75.0 °C	74.9 °C	0.1 °C	Passed
PT1000, 100 °C	100.0 °C	99.9 °C	0.1 °C	Passed

## Summary of Certification

Certification of instrument

**Passed**

The instrument referred to in this certificate has fulfilled the criteria of the certification. This is indicated by the notation Passed in the column above.

Remarks - Test high impedance at 1900.0 mV, Results : 1899.8 mV

Difference = 0.005% Within MPE (0.033%)

Certification of the instrument was performed by

Name Khomsan Pralaung Function Service

Place Mettler-Toledo (Thailand) Ltd.

Calibration Date: 29-Jan-2025

Signature

**COPY**

Mettler-Toledo (Thailand) Limited

# METTLER TOLEDO

## Performance Test

Attachment to Certificate No. CCP-0403-25

## pH Electrode

Type **InLab Expert Pro-ISM** S/N: **2463982**

## Certified standards used

Standard 1:	Type: pH Buffer	Manufacturer: METTLER TOLEDO	Exp. date: 3-Dec-2026
	Nominal value: pH ( 25.00 °C):	4.01	Lot No.: 1J338E
Standard 2:	Type: pH Buffer	Manufacturer: METTLER TOLEDO	Exp. date: 27-Nov-2026
	Nominal value: pH ( 25.00 °C):	7.00	Lot No.: 1J331B
Standard 3:	Type: pH Buffer	Manufacturer: METTLER TOLEDO	Exp. date: 11-Jan-2026
	Nominal value: pH ( 25.00 °C):	10.00	Lot No.: 1K011B
Standard 4:	Type: Redox Solution	Manufacturer: METTLER TOLEDO	Exp. date: -
	Nominal value: pH ( 25.00 °C):	-	Lot No.: -

## Adjustment

Set Calibration Buffer	B1 (25 °C) 1.68, 4.01, 7.00, 10.01					
Select Calibration Mode	3-Point calibration		2-Point calibration		2-Point calibration	
Segment	°C	pH	°C	pH	°C	pH
Cal 1	ATC 25.5	7.00	ATC		ATC	
Cal 2	ATC 25.5	4.00	ATC		ATC	
Offset (mV)	-27.2					
Slope % (or mV/pH)	95.9					
Cal 3	ATC 25.5	10.01				
Offset (mV)	-27.2					
Slope % (or mV/pH)	97.4					

## Measurements

Resolution: 2 Decimal places

As Found					As Left				
Buffer Values	Measured		Difference		Buffer Values	Measured		Difference	
pH	°C	pH	pH		pH	°C	pH	pH	
4.01	25.3	ATC	4.02	0.01	4.01	25.3	ATC	4.01	0.00
7.00	25.2	ATC	6.98	-0.02	7.00	25.2	ATC	7.01	0.01
9.99	25.3	ATC	10.11	0.12	9.99	25.2	ATC	10.00	0.01

Redox Measurement Result = - mV

Note: The difference result of calibrated electrode should be within +/- 0.05 pH

Remarks: N/A

Place: Laboratory

Calibration Date: 29-Jan-2025

Service Specialist: Khomsan Pralaung

Signature:

**COPY**

**STANDARD WEIGHT 50 g**

Certificate No. : 24-062445  
Sample Code : 24-25551-001

## CERTIFICATE OF CALIBRATION

Customer : EASTERN THAI CONSULTING 1992 CO., LTD.  
683 Moo 11, Sukhapibarn 8 Rd., Nongkham,  
Sriracha, Chonburi 20230

Location of Calibration : Asia Medical and Agricultural Laboratory and Research Center Public Company Limited  
(Calibration Laboratory)

Equipment : Standard Weight 50 g

Manufacturer : METTLER TOLEDO

Class : F1

Serial No. : N/A

ID No. : LABE 10/1

Date of Receipt : 23 May 2024

Date of Calibration : 03 June 2024

Calibrated by Mr. Somwang Sangdee  
Scientist

Approved by ( Mr. Somchai Neampunt )  
Signed for Director

Issue date 04 June 2024

The uncertainties are for a confidence probability of approximately 95%.

The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Asia Medical and Agricultural Laboratory and Research Center Public Company Limited (AMARC).

Certificate No. : 24-062445  
Sample Code : 24-25551-001

## REPORT OF CALIBRATION

Equipment : Standard Weight 50 g  
Manufacturer : METTLER TOLEDO  
Class : F1  
Serial No. : N/A  
ID No. : LABE 10/1

## Result of Calibration :

☒ Without adjustment☐ Adjustment

Conventional value of the result of weighing in air. For a weight taken at a reference temperature ( $t_{ref}$ ) of 20°C, the conventional mass is the mass of a reference weight of a density ( $\rho_{ref}$ ) of 8000 kg.m<sup>-3</sup> which it balances in air of a reference density ( $\rho_a$ ) of 1.2 kg.m<sup>-3</sup>

Description	Deviation	Conventional Mass	Expanded Uncertainty	Maximum Permissible Error	ID No.
	(mg)		(mg)	± (mg)	
50 g	-0.343	49.999657 g	0.10	0.30	LABE 10/1

The result expanded uncertainty of measurement  $U$  is stated as the standard uncertainty of measurement multiplied by the coverage factor  $k = 2.0$ , which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty of measurement has been determined in accordance with UKAS M3003

COPY



Certificate No. : 24-062445

Sample Code : 24-25551-001

## REPORT OF CALIBRATION

## Condition of Calibration

1. Ambient Conditions : Temperature  $20^{\circ}\text{C} \pm 1.5^{\circ}\text{C}$ , Relative humidity  $50\% \pm 10\%$  and air density  $1.19 \text{ kg/m}^3$ 

2. Calibration Method : Direct comparison weighing according to OIML R111-1 : 2004(E)

3. Reference standard instrument

Instrument	Class	ID No.	Certificate No.	Due Date
1) Standard Weight 1 mg to 1 kg	E2	LB-WE-83	24-001894	11 January 2025

4. This certification is traceable to the International System of Unit maintained at : -

Asia Medical and Agricultural Laboratory and Research Center Public Company Limited

(Instrument number 1).

5. Condition of Calibration item: Normal

## 6. Description of Calibrated Item :

Type and Nominal Value :	Standard Weight 50 g
Shape :	Cylindrical weight with knob
Material :	Stainless steel
Case :	Wooden Box
Comments :	Recalibration

- End of Report -

COPY

**STANDARD WEIGHT 100 g**





Certificate No. : 24-079772  
Sample Code : 24-31841-002

## CERTIFICATE OF CALIBRATION

Customer : EASTERN THAI CONSULTING 1992 CO., LTD.  
683 Moo 11, Sukhapibarn 8 Rd., NongKham,  
Sriracha, Chonburi 20230

Location of Calibration : Asia Medical and Agricultural Laboratory and Research Center Public Company Limited  
(Calibration Laboratory)

Equipment : Standard Weight 100 g

Manufacturer : N/A

Class : N/A

Serial No. : N/A

ID No. : LABE 10/2

Date of Receipt : 25 June 2024

Date of Calibration : 30 June 2024

Calibrated by Mr. Nawa Sisuwan  
Scientist

Approved by ( Mr. Somchai Neampunt )  
Signed for Director

Issue date 03 July 2024

The uncertainties are for a confidence probability of approximately 95%.

The calibration result is applied only to the above calibrated item and was found accurate as shown on date and photo of calibration only.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Asia Medical and Agricultural Laboratory and Research Center Public Company Limited (AMARC).



Certificate No. : 24-079772  
Sample Code : 24-31841-002

## REPORT OF CALIBRATION

Equipment : Standard Weight 100 g  
Manufacturer : N/A  
Class : N/A  
Serial No. : N/A  
ID No. : LABE 10/2

Result of Calibration : ☒ Without adjustment ☐ Adjustment

Conventional value of the result of weighing in air. For a weight taken at a reference temperature ( $t_{ref}$ ) of 20°C, the conventional mass is the mass of a reference weight of a density ( $\rho_{ref}$ ) of 8000 kg.m<sup>-3</sup> which it balances in air of a reference density ( $\rho_a$ ) of 1.2 kg.m<sup>-3</sup>

Description	Deviation	Conventional Mass	Expanded Uncertainty	Maximum Permissible Error	ID No.
	(mg)		(mg)	± (mg)	
100 g	-0.173	99.999827 g	0.16	0.50	LABE 10/2

The result expanded uncertainty of measurement  $U$  is stated as the standard uncertainty of measurement multiplied by the coverage factor  $k = 2.0$ , which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty of measurement has been determined in accordance with UKAS M3003



Certificate No. : 24-079772  
Sample Code : 24-31841-002

## REPORT OF CALIBRATION

### Condition of Calibration

1. Ambient Conditions : Temperature  $20^{\circ}\text{C} \pm 1.5^{\circ}\text{C}$ , Relative humidity  $50\% \pm 10\%$  and air density  $1.19 \text{ kg/m}^3$

2. Calibration Method : WI-CL-007 base on OIML R 111-1 : 2004(E)

3. Reference standard instrument

Instrument	Class	ID No.	Certificate No.	Due Date
1) Standard Weight 1 mg to 1 kg	E2	LB-WE-83	24-001894	11 January 2025

4. This certification is traceable to the International System of Unit maintained at : -

Asia Medical and Agricultural Laboratory and Research Center Public Company Limited

(Instrument number 1).

5. Condition of Calibration item: Normal

### 6. Description of Calibrated Item :

Type and Nominal Value :	Standard Weight 100 g
Shape :	Cylindrical weight with knob
Material :	Stainless steel
Case :	Wooden Box
Comments :	Recalibration

- End of Report -

COPY

**STANDARD WEIGHT 50 g**



Certificate No. : 24-079773  
Sample Code : 24-31841-003

## CERTIFICATE OF CALIBRATION

Customer : EASTERN THAI CONSULTING 1992 CO., LTD.  
683 Moo 11, Sukhapibarn 8 Rd., NongKham,  
Sriracha, Chonburi 20230

Location of Calibration : Asia Medical and Agricultural Laboratory and Research Center Public Company Limited  
(Calibration Laboratory)

Equipment : Standard Weight 50 g

Manufacturer : N/A

Class : N/A

Serial No. : N/A

ID No. : LABE 10/4

Date of Receipt : 25 June 2024

Date of Calibration : 30 June 2024

Calibrated by Mr. Nawa Sisuwan  
Scientist

Approved by ( Mr. Somchai Neampunt )  
Signed for Director

Issue date 03 July 2024

The uncertainties are for a confidence probability of approximately 95%.

The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Asia Medical and Agricultural Laboratory and Research Center Public Company Limited (AMARC).



Certificate No. : 24-079773  
Sample Code : 24-31841-003

## REPORT OF CALIBRATION

Equipment : Standard Weight 50 g

Manufacturer : N/A

Class : N/A

Serial No. : N/A

ID No. : LABE 10/4

Result of Calibration : ☒ Without adjustment ☐ Adjustment

Conventional value of the result of weighing in air. For a weight taken at a reference temperature ( $t_{ref}$ ) of 20°C, the conventional mass is the mass of a reference weight of a density ( $\rho_{ref}$ ) of 8000 kg.m<sup>-3</sup> which it balances in air of a reference density ( $\rho_0$ ) of 1.2 kg.m<sup>-3</sup>

Description	Deviation	Conventional Mass	Expanded Uncertainty	Maximum Permissible Error	ID No.
	(mg)		(mg)	± (mg)	
50 g	-0.176	49.999824 g	0.10	0.30	LABE 10/4

The result expanded uncertainty of measurement  $U$  is stated as the standard uncertainty of measurement multiplied by the coverage factor  $k=2.0$ , which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty of measurement has been determined in accordance with UKAS M3003

Certificate No. : 24-079773

Sample Code : 24-31841-003

## REPORT OF CALIBRATION

## Condition of Calibration

1. Ambient Conditions : Temperature  $20^{\circ}\text{C} \pm 1.5^{\circ}\text{C}$ , Relative humidity  $50\% \pm 10\%$  and air density  $1.19 \text{ kg/m}^3$
2. Calibration Method : WI-CL-007 base on OIML R 111-1 : 2004(E)
3. Reference standard instrument

Instrument	Class	ID No.	Certificate No.	Due Date
1) Standard Weight 1 mg to 1 kg	E2	LB-WE-83	24-001894	11 January 2025

4. This certification is traceable to the International System of Unit maintained at : -

Asia Medical and Agricultural Laboratory and Research Center Public Company Limited

( Instrument number 1).

5. Condition of Calibration item: Normal

## 6. Description of Calibrated Item :

Type and Nominal Value :	Standard Weight 50 g
Shape :	Cylindrical weight with knob
Material :	Stainless steel
Case :	Wooden Box
Comments :	Recalibration

- End of Report -



COPY

**SPECTROPHOTOMETER**

**Model : PROVE 100**

**Serial No. : 1613110857**



## CERTIFICATE OF CALIBRATION

**Instrument** : SPECTROPHOTOMETER  
**Model** : PROVE 100  
**Date of Calibration** : February 07, 2025  
**Customer Name** : Eastern Thai Consulting 1992 Co., Ltd.

### Procedure used.

The wavelength accuracy and the linearity of the absorbance measurement of photometers are checked using Check solutions according to Merck calibration laboratory work instruction.

### Measurements results

**Function** : **Photometric Accuracy** Absorbance measurement.  
All data shown below as received values of blank solution before adjustment.

Check Solution (Abs.)	Wavelength (nm)	Desired Absorbance (Abs.)	Measured Absorbance (Abs.)	Error (Abs)
0.000	445	0.000 ± 0.005	0.000	0.000
0.000	525	0.000 ± 0.005	0.000	0.000
0.000	690	0.000 ± 0.005	0.000	0.000

CERTIFICATE No. **WO-02931344**



Merck Ltd. Thailand

19<sup>th</sup> Floor, Emporium Tower, 622 Sukhumvit Road  
Klongton, Klongtoey, Bangkok 10110  
Tel. : +66 (0) 2667 8000  
Fax : +66 (0) 2667 8399

Customer Care Center : +66 (0) 2667 8333

www.merck.co.th

1 of 4

**COPY**



## CERTIFICATE OF CALIBRATION

**Function** : **Photometric Accuracy** Absorbance measurement.  
All data shown below were final value of standard solution after adjustment.

Check Solution (Abs.)	Desired Absorbance (Abs.)	Allowed tolerance. (Abs.)	Actual Absorbance (Abs.)	Assessment Yes/No
445-1	0.197	± 0.020	0.193	Yes
445-2	0.497	± 0.030	0.491	Yes
445-3	0.990	± 0.040	0.979	Yes
445-4	1.494	± 0.050	1.479	Yes
525-1	0.198	± 0.020	0.198	Yes
525-2	0.493	± 0.030	0.491	Yes
525-3	0.988	± 0.040	0.975	Yes
525-4	1.485	± 0.050	1.468	Yes
690-1	0.204	± 0.020	0.202	Yes
690-2	0.504	± 0.030	0.495	Yes
690-3	0.987	± 0.040	0.995	Yes
690-4	1.498	± 0.050	1.496	Yes

\* Spectroquant Photo check (Check Solution) **Lot: HC299606**

- Check solution for this certification is traceable to: Reference Photometer Agilent Cary 4000 checked and calibrated using NIST-grey glass filter SRM 1930 and Holmium oxide Solution NIST SRM 2034  
- Desired absorbance round cell has been calculated from the absorbance of the 1 cm cell using the path length of the round cell and is entered as the desired



Merck Ltd. Thailand

19<sup>th</sup> Floor, Emporium Tower, 622 Sukhumvit Road  
Klongton, Klongtoey, Bangkok 10110  
Tel. : +66 (0) 2667 8000  
Fax : +66 (0) 2667 8399

Customer Care Center : +66 (0) 2667 8333

www.merck.co.th

2 of 4

**COPY**





## CERTIFICATE OF CALIBRATION

Software version: 2.0.1

Wavelength Accuracy				
Equipment	Nominal value	Tolerance limit	Actual value	Result
Holmium Oxide Liquid Filter Hellma 667-UV5	361.25 nm	360.05 - 362.45 nm	361.0 nm	P
	451.35 nm	450.15 - 452.55 nm	451.3 nm	P
	485.25 nm	484.05 - 486.45 nm	485.0 nm	P
	536.60 nm	535.40 - 537.80 nm	537.6 nm	P
	640.50 nm	639.30 - 641.70 nm	641.2 nm	P
Stray Light				
Equipment	Wavelength	Nominal value	Actual value	Result
Sodium Nitrite Hellma 667-UV11	340 nm	≤0.10 %T	0.05 %T	P
Self-test Hardware				P
No visual flaws, no burrs, no loose parts, and fastenings				

3 of 4



Merck Ltd. Thailand  
19<sup>th</sup> Floor, Emporium Tower, 622 Sukhumvit Road  
Klongton, Klongtoey, Bangkok 10110  
Tel : +66 (0) 2667 8000  
Fax : +66 (0) 2667 8399  
Customer Care Center : +66 (0) 2667 8333

www.merck.co.th

COPY



## CERTIFICATE OF CALIBRATION

INSTRUMENT : SPECTROPHOTOMETER

MANUFACTURER : Merck KGaA, Darmstadt, Germany

MODEL : PROVE 100

SERIAL No. : 1613110857

CLIENT : Eastern Thai Consulting 1992 Co., Ltd.

DATE OF ISSUE : February 07, 2025

## APPROVED SIGNATORY

NAME : Mr.Supachai Konthong  
(INSTRUMENTAL SERVICE ENGINEER)

SIGNATURE : \_\_\_\_\_

This certificate may not be reproduced except in full unless permission for the reproduction has been obtained in writing from the laboratory.

CERTIFICATE No. **WO-02931344**



Merck Ltd. Thailand  
19<sup>th</sup> Floor, Emporium Tower, 622 Sukhumvit Road  
Klongton, Klongtoey, Bangkok 10110  
Tel : +66 (0) 2667 8000  
Fax : +66 (0) 2667 8399  
Customer Care Center : +66 (0) 2667 8333

www.merck.co.th

4 of 4

COPY

**THERMO-HYGROMETER**

**Model : 608-H1**

**Serial No. : 45106737**

## CERTIFICATE OF CALIBRATION

Certificate No. : 25-090091

Sample Code : 25-39161-001

Customer : EASTERN THAI CONSULTING 1992 CO., LTD.  
683 Moo 11, Sukhapiarn 8 Rd., Nongkham,  
Sriracha, Chonburi 20230

Location of Calibration : Asia Medical and Agricultural Laboratory and Research Center Public Company Limited  
(Calibration laboratory)

Equipment : Digital thermo-hygrometer

Manufacturer : testo Model : 608-H1

Serial No. : 45106737 ID No. : LABE 09/7

Date of Receipt : 21 May 2025 Date of Calibration : 23 May 2025

## Condition of Calibration

1. Environment 1.1 Ambient temperature : 23.0 °C ± 3.0 °C  
1.2 Relative humidity : 55.0 % ± 15.0 %

## 2. Calibration method

- 2.1 In-house method: WI-CL-045 By comparison with thermometer standard / chilled mirror hygrometer in controlled chamber.  
2.2 The calibration by comparison unit under calibration (UUC) to the thermometer standard / chilled mirror hygrometer in a chamber at the controlled temperature / relative humidity.

## 3. Reference standard instrument

Instrument	Model	ID No.	Certificate No.	Due Date
3.1 Chilled Mirror	Optidew 401	LB-DP-03 & LB-DP-03 (DP)	TH-0122-24	25 September 2025
3.2 Digital Thermometer	Optidew 401	LB-DP-03 & LB-DP-03 (Temp.)	24-138856	28 October 2025
3.3 Digital Thermometer	34972A	LB-DA-07 with RTD-89	24-106857	21 August 2025

## 4. This certificate is traceable to the international system of unit (SI Unit).

- 4.1 Instrument No. 3.1 through National Institute of Metrology (Thailand).  
4.2 Instrument No. 3.2 and 3.3 through Asia Medical and Agricultural Laboratory and Research Center Public Company Limited.

## 5. This result of calibration was found accurate as shown on date and place of calibration only.

## 6. Condition of calibration item : Normal

Calibrated by Miss Pornsuda Lohabal

Scientist

Approved by

(Mr. Somchai Neampunt)

Signed for Director

Issue date 26 May 2025

The uncertainties are for a confidence probability of approximately 95%.

The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Asia Medical and Agricultural Laboratory and Research Center Public Company Limited (AMARC).

## REPORT OF CALIBRATION

Certificate No. : 25-090091

Sample Code : 25-39161-001

## Results of Calibration

## Temperature measurement

Resolution : 0.1 °C  
Range : 0 °C to 50 °C

Calibration point °C	Average of standard reading		Unit under calibration		uncertainty °C
	Controlled humidity %RH	Temperature °C	Average reading °C	Correction value °C	
20	50	20.01	20.2	- 0.19	± 0.39
25	50	25.01	25.0	+ 0.01	± 0.39
30	50	30.01	30.0	+ 0.01	± 0.39

## Humidity measurement

Resolution : 0.1 %RH  
Range : 10 %RH to 95 %RH

Calibration point %RH	Average of standard reading		Unit under calibration		uncertainty %RH
	Air temperature °C	Calculated humidity %RH	Average reading %RH	Correction value %RH	
45	25.02	45.10	50.2	- 5.10	± 1.3
60	25.02	60.15	65.2	- 5.05	± 1.5
75	25.02	75.01	82.1	- 7.09	± 1.7

## Notes

- Calibration results without adjustment.

The result expanded uncertainty of measurement  $U$  is stated as the standard uncertainty of measurement multiplied by the coverage factor  $k=2.00$ , which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty of measurement has been determined in accordance with UKAS M3003.

- End of Report -

COPY

COPY

**UV/VIS SPECTROPHOTOMETER**

**Model : UV-1800**

**Serial No. : A11635101643 CD**

# Certificate of Calibration

Number of Page(s) 1 of 3

**Certificate No.** BSCC-UV-153/25  
**Equipment** UV/Vis Spectrophotometer  
**Model** UV-1800  
**Manufacturer** Shimadzu  
**Serial No.** A11635101643 CD  
**ID No.** LABC 03/2  
**Date of receipt** 21 April 2025  
**Date of calibration** 21 April 2025  
**Date of issue** 25 April 2025

**Customer name** Eastern Thai Consulting 1992 Co., Ltd.

**Address** 683 Moo 11, Sukkaphibarn 8 Rd., Nongkham, Sriracha, Chonburi 20230

**Temperature** (24.7-26.8) °C (On site)  
**Humidity** (36.9-46.2) %RH (On site)

**Equipment condition** Good Operation

**Calibration Location** Analysis Department

**Calibration Procedure** In-house method WI-UV-702-01 based on ASTM E275-01

**Traceability** Wavelength Accuracy is traceable to certificate No. 114485 and 114511  
Photometric Accuracy is traceable to certificate No. 119612 and 114653  
Stray Light is traceable to certificate No. 114484  
The above certificate are traceable to SI unit through Sarna Scientific Ltd.  
(UKAS accredited calibration laboratory NO. 0659)

**Calibrated by** Mr.Phongpak Sonbunchu

Approved by



**Mr. Panhaphong Phanmekakul**  
Technical Manager

**COPY**

The above results are valid exclusively for the calibrated item(s) as mention in this report / certificate.  
Advertising the report / Certificate and publicity of the results are prohibited and also shall not be reproduced  
except in full, without written approval of the Bara Scientific Co., Ltd.

# Certificate of Calibration

**Certificate No.** BSCC-UV-153/25

Number of Page(s) 2 of 3

**Calibration Results:**

**1.Wavelength Accuracy**

Certified Wavelength (nm)	UUC (nm)	Error (nm)	Uncertainty (±nm)
287.71	287.70	-0.01	0.18
445.82	445.87	0.05	0.18
536.52	536.52	0.00	0.18
741.02	741.05	0.03	0.18
879.41	879.33	-0.08	0.18

**2.Photometric Accuracy (UV)**

Wavelength (nm)	Certified Absorbance (A)	UUC (A)	Error (A)	Uncertainty (±A)
235	0.0000	-0.0001	-0.0001	0.0075
	0.7404	0.7416	0.0012	0.0075
257	CNR	CNR	CNR	CNR
	CNR	CNR	CNR	CNR
313	CNR	CNR	CNR	CNR
	CNR	CNR	CNR	CNR
350	0.0000	0.0000	0.0000	0.0075
	0.6397	0.6398	0.0001	0.0075

\*CNR = Customer not request

**COPY**

The above results are valid exclusively for the calibrated item(s) as mention in this report / certificate.  
Advertising the report / Certificate and publicity of the results are prohibited and also shall not be reproduced  
except in full, without written approval of the Bara Scientific Co., Ltd.



**Bara Scientific Co., Ltd.**  
968 U Chu Liang Building Floor7 Rama4 Road  
Silom Bangkok Bangkok Thailand 10500  
Tel : 02-6324300 Fax : 02-6375496-7  
www.barascientific.com



# Certificate of Calibration

Certificate No. BSCC-UV-153/25

Number of Page(s) 3 of 3

## Calibration Results:

### 3. Photometric Accuracy (Visible)

Wavelength (nm)	Certified Absorbance (A)	UUC (A)	Error (A)	Uncertainty ( $\pm A$ )
420.0	0.0000	0.0001	0.0001	0.0042
	0.5733	0.5712	-0.0021	0.0042
	0.7113	0.7097	-0.0016	0.0042
	1.0164	1.0150	-0.0014	0.0042
440.0	0.0000	0.0000	0.0000	0.0042
	0.5581	0.5559	-0.0022	0.0042
	0.6996	0.6975	-0.0021	0.0042
	1.0000	0.9984	-0.0016	0.0042
465.0	CNR	CNR	CNR	CNR
	CNR	CNR	CNR	CNR
	CNR	CNR	CNR	CNR
	CNR	CNR	CNR	CNR
546.1	0.0000	0.0000	0.0000	0.0042
	0.5217	0.5202	-0.0015	0.0042
	0.6970	0.6947	-0.0023	0.0042
	0.9982	0.9969	-0.0013	0.0042
590.0	CNR	CNR	CNR	CNR
	CNR	CNR	CNR	CNR
	CNR	CNR	CNR	CNR
	CNR	CNR	CNR	CNR
635.0	0.0000	0.0000	0.0000	0.0042
	0.5630	0.5620	-0.0010	0.0042
	0.7615	0.7594	-0.0021	0.0042
	1.0953	1.0943	-0.0010	0.0042

\*CNR = Customer not request

### 4. Stray Light\*

Standard cut-off wavelength (nm)	Unit Under Calibration(UUC)		
	Wavelength (nm)	Transmission (%T)	Absorbance (A)
201.10 $\pm$ 0.11nm	200.85	0.9740	2.0116

The Stray light transmission reference is less than 1.0%T and Stray light absorbance reference is greater than 2.00A

\*Stray Light not NSC-ONSC Accredited.

The measurement uncertainty is base on a standard uncertainty multiplied by a coverage factor k=2 providing a level of confidence of approximately 95%.

\*\*\*End of Certificate\*\*\*

**COPY**

The above results are valid exclusively for the calibrated item(s) as mention in this report / certificate.  
Advertising the report / Certificate and publicity of the results are prohibited and also shall not be reproduced  
except in full, without written approval of the Bara Scientific Co., Ltd.



## Agilent CrossLab Start Up Services

# Agilent 7890 Gas Chromatograph Preventive Maintenance Checklist

Agilent Preventive Maintenance provides factory recommended service for your analytical instruments to assure reliable operation and the accuracy of your results.

Delivered by highly trained and certified service engineers using genuine Agilent parts and supplies, Agilent Preventive Maintenance provides everything you need to reduce unplanned downtime and keep your systems operating at their peak. This checklist will be completed at the end of the service and provided to you as a record of the preventive maintenance activities.

## Agilent 7890 GC Preventive Maintenance Checklist

### Introduction

### Customer Information

- Customers should provide all necessary operating supplies upon request of the engineer.
- A customer representative should be available to the engineer while performing the preventive maintenance procedures.
- Any parts, not included in the Parts Lists section of this document, are not part of the recommended Preventive Maintenance service, nor are they included in the price of this service.
- If a system requires the use of extra or special procedures and/or parts for the maintenance service, then these must be ordered separately and charged as a repair, which may incur additional costs.

### Important Customer Web Links

- For more information about **Agilent Technologies services**, please visit our website using the following URL: <http://www.agilent.com/en-us/products/crosslab-instrument-services/service-repair>
- The **Agilent Community** is an excellent place to get answers, collaborate with others about applications and Agilent products, and find in-depth documents and videos relevant to Agilent technologies. Visit <https://community.agilent.com/welcome>.
- To access **Agilent University**, visit <http://www.agilent.com/crosslab/university/> to learn about training options, which include online, classroom and onsite delivery. A training specialist can work directly with you to help determine your best options.
- A useful **Agilent Resource Center** web page is available, which includes short videos on maintenance, quick lists of consumables for new instruments, and other valuable information. Check out the Resource Page here: <https://www.agilent.com/en-us/agilentresources>.
- Need technical support, FAQs, supplies? – Visit our **Support Home page** <http://www.agilent.com/search/support>.
- **Videos** about specific preparation requirements for your instrument can be found by searching the **Agilent YouTube** channel at <https://www.youtube.com/user/agilent>.
- **7890B Manuals** are also available on Agilent.com:
  - **Safety** [https://www.agilent.com/cs/library/usermanuals/public/7890B\\_Safety.pdf](https://www.agilent.com/cs/library/usermanuals/public/7890B_Safety.pdf)
  - **Installation and First Startup** [https://www.agilent.com/cs/library/usermanuals/Public/7890B\\_Installation.pdf](https://www.agilent.com/cs/library/usermanuals/Public/7890B_Installation.pdf)
  - **Operation Manual** [https://www.agilent.com/cs/library/usermanuals/Public/7890B\\_Operation.pdf](https://www.agilent.com/cs/library/usermanuals/Public/7890B_Operation.pdf)
  - **Maintaining Your GC** [https://www.agilent.com/cs/library/usermanuals/public/G3430-90052%207890B\\_Maintaining%20Guide.pdf](https://www.agilent.com/cs/library/usermanuals/public/G3430-90052%207890B_Maintaining%20Guide.pdf)



## Service Engineer's Responsibilities

- Contact the customer and ensure that all necessary supplies are available before the preventive maintenance visit.
- Only select those pages that relate to the system or module being serviced.
- Complete empty fields with the relevant information.
- Complete the relevant checkboxes in the checklist using either a "X" or tick mark "✓".
- Check "Section not applicable" check boxes to indicate services/tasks not delivered, as appropriate.
- Complete the Preventive Maintenance service in the order of the tasks listed.
- Complete the Service Review section together with the customer.
- Complete the fields for page numbers at the foot of each selected page
- Complete the total number of pages field in the Service Completion section
- **Ask the customer to sign the Service Completion section including the customer's and your signature.**

## Additional Instruction Notes

- Check for any active service notes for this unit. If there are any applicable "Safety" or "Modification Recommended" Service notes, plan to implement the changes on this unit before doing any qualification service.
- Do not implement firmware updates, unless you get approval from the customer and are sure that they are compatible with the instrument control software.

## System Information

- ☒ Check this box if an instrument configuration report is attached instead of completing the table below.

Instrument System Name and ID	GC7890B	CN15343147
Instrument System Site and Location	Sect Co, Ltd. Instrument room.	

List System Component Product Numbers	List the Serial Numbers of each Component
1. G7440B	CN15343147
2. G4519A	CN1910080
3. G4514A	CN19080006
4.	
5.	
6.	
7.	
8.	
9.	
10.	

## Preparation

- ☒ Discuss any specific issues with the customer before starting.
- ☒ Review the instrument logbook for recorded problems and comments.
- ☒ Save instrument control settings before starting the procedure.
- ☒ Perform a general inspection of the system for cleanliness.
- ☒ Check for proper installation of parts, assemblies, sensors etc.
- ☒ Check system for required installation of components, settings as defined by current Service Notes.
- ☒ Check for required firmware updates and verify with customers if they would like them installed.
- ☒ Before starting the following procedures, record the Detector Signal Output(s) in the results table. If the GC is turned OFF or in a service mode, comparing the detector outputs before and after the service is not possible.

## Preventive Maintenance Procedure

### Clean and inspect GC

- ☒ Unplug power cord from the power source.
- ☒ Open GC covers and vacuum/remove any dust/debris. Pay particular attention to cooling fans.
- ☒ Inspect internal connectors for proper contact and placement.
- ☒ Reconnect Power to the GC. Power the GC on and verify the power on self-test passed.
- ☒ Verify oven motor spins freely and turns on with the oven door closed; off when the door is opened.
- ☒ Verify operation of all other fans - the inlet and EPC cooling fans.
- ☒ Verify oven intake/outlet flap assembly is operating smoothly while heating and cooling the oven

### Inlet and detector consumable replacement

- ☒ For the inlets installed, perform inlet maintenance as defined in the 7890 manual – "Maintaining Your GC" - for the inlet(s) installed.
- ☒ Replace the split vent trap cartridge filter on units with these inlets: Split/Splitless Capillary (SSL), Multi-Mode Inlet (MMI), Programmed Temperature Vaporizer (PTV), Volatiles Interface (VI).
- ☒ If the inlet system is used in Split Mode with viscous samples, inspect and clean the split vent tube on the inlet and flush or replace the tubing between the inlet and the split vent trap.
- ☒ If the GC includes a Flame Ionization Detector (FID), replace the jet. If the ignitor shows any buildup of sample or corrosion, replace the ignitor. Examine the FID collector and castle assemblies for contamination – clean as necessary.

### Zero Sensors and Leak test

- ☒ Zero all pressure sensors per the procedure in the 7890 "Advanced User Guide".
- ☒ Perform inlet pressure decay test(s) as defined in the 7890 "Troubleshooting Manual". If the PM is done in preparation for an Operational Qualification, then the pressure decay test defined within that protocol can be used for the PM.
- ☒ Record if test passed or failed in the results table.

## ALS Maintenance

- ☐ **Section NOT applicable**
- ☒ Check all cabling and configuration settings between GC, tray, and injectors.
- ☒ Vacuum or remove any dust, especially around fans.
- ☒ Check operation of all fans.
- ☒ Check syringe for smooth plunger operation.
- ☒ Check for smooth operation of the needle support – clean if necessary

## Restore Instrument

- ☒ Restore the normal operating conditions or customer method using the Data System.
- ☒ Purge the system with carrier flow for 15 minutes
- ☒ Bake out the system, then restore the normal operating conditions
- ☒ After equilibration, check and record the post PM detector signal output values. Results should be similar or lower than the detector outputs recorded prior to PM.
- ☐ Perform a chemical checkout. If this is a routine PM, inject the customer's sample using the ALS if applicable. This will act as a final checkout of both the ALS and the GC.

Note: If the PM Service is performed prior to a qualification service, then use the qualification procedure as a guide for final instrument set up and checkout.

## Signature Page

### Service Review

- ☐ Attach available reports/printouts of all tests to this documentation.
- ☒ Record the Preventive Maintenance service activity in the customer's records/logbook.
- ☒ Update/reset instrument maintenance counters as appropriate.
- ☒ Affix the PM sticker to the system or instrument logbook based on the customer's request.
- ☒ Complete the Service Engineer Comments section if there are additional comments.
- ☒ Review with the customer this service, parts replaced, and test results obtained.
- ☒ If the instrument firmware was updated, record the details of the change in the Service Engineer's Comments box or if necessary, in the customer's IQ records.
- ☐ Supply the customer with a copy of the Smart Alerts flyer.
- ☐ Describe Smart Alerts to the customer.
- ☐ Install Smart Alerts if requested.

## 7890 GC Test Results Table

Detector Signal Outputs	Before PM Service	After PM Service
Front detector output <i>100</i>	<i>N/A</i>	<i>126.2</i>
Back detector output <i>FID</i>	<i>N/A</i>	<i>22.6</i>
AUX detector output	<i>N/A</i>	<i>N/A</i>
<b>Pressure decay test</b>	<b>Expected test result</b>	<b>Actual test result</b>
Front inlet pressure decay test	Pass	<i>Pass</i>
Back inlet pressure decay test	Pass	<i>Pass</i>

## 7890 Parts List Table

The following kits are recommended for capillary and purged packed inlets. If this is a general PM and the customer has a preferred set of consumables, you may use the customer's consumables.

Part description	Part number	Product or model# where used	Quantity consumed
SSL Capillary Inlet PM kit, Splitless	5188-6497	7890A/B	<i>N/A</i>
SSL Capillary Inlet PM kit, split	5188-6496	7890A/B	<i>2</i>
SSL Capillary Ultra Inert Inlet Gold Seal with Washer	5190-6144	7890A/B	<i>N/A</i>
SSL Capillary Ultra Inert Inlet Splitless Liner - Single taper with Glass Wool	5190-2293	7890A/B	<i>N/A</i>
SSL Capillary Ultra Inert Inlet Low Pressure Drop Split Liner - with Glass Wool	5190-2295	7890A/B	<i>N/A</i>
PP Inlet PM kit	5188-6498	7890A/B	<i>N/A</i>
Split vent trap PM kit, single cartridge (for MMI, PTV & VI)	5188-6495	7890A/B	<i>N/A</i>
MMI Cleaning Kit	G3510-60820	7890A/B	<i>N/A</i>
PTV Septumless Head Rebuild Kit	5182-9747	7890A/B	<i>N/A</i>
PTV Septumless Head Teflon Guide	5182-9748	7890A/B	<i>N/A</i>
Ignitor (glow plug) assembly with O-ring	19231-60680	7890A/B	<i>1</i>
FID Collector Rebuild/Cleaning Kit	G1531-67000	7890A/B	<i>N/A</i>
Standard .011-inch FID Jet for capillary FID base	G1531-80560	7890A/B	<i>1</i>
High Temperature .018-inch FID Jet for capillary FID base	G1531-80620	7890A/B	<i>N/A</i>
Standard .018-inch FID Jet for packed column with packed FID base	18710-20119	7890A/B	<i>N/A</i>
Standard .011-inch FID Jet for capillary column with packed/adaptable FID base	19244-80560	7890A/B	<i>N/A</i>
High Temperature .018-inch FID Jet for capillary column with packed/adaptable FID base	19244-80620	7890A/B	<i>N/A</i>
NPD Jet, universal fit, .011-inch ID	G1534-80580	7890A/B	<i>N/A</i>
NPD Jet, universal fit, .011-inch ID Extended tip	G1534-80590	7890A/B	<i>N/A</i>
SSL Capillary Ultra Inert Inlet Gold Seal with Washer	5190-6144	7890A/B	<i>N/A</i>
SSL Capillary Ultra Inert Inlet Splitless Liner - Single taper with Glass Wool	5190-2293	7890A/B	<i>N/A</i>
**FID Collector Replacement Kit, if needed	G1531-67001	7890A/B	<i>N/A</i>



## Certificate of Completion

Learner Name: Saenguthai Saeng Tarak

Title Of Course: AN-ASP/CE/CSE-GC-1-001-M: 7890/7820 GC and OL GC Standalone Chemstation I&F/Service

Completion Date: November 23, 2014

Certified By Company: Learning at Agilent

**All Service and Support training certificates have the following specific limitations.**

A certificate for Service and Support training is only valid while employed by Agilent Technologies or while working as an Agilent-authorized service provider, through which the service employee has ongoing access to Agilent's: Safety Alerts, Service Notes, internal technical updates, update training, current documentation, technical support, current parts, and parts updates. Completion of training alone, without being employed by Agilent Technologies, does not qualify an individual to safely install, service or maintain Agilent products.

### Service Engineer Comments

If there are any specific points you wish to note as part of performing the service or other items of interest for the customer, please write include them in this box.

### Service Completion

Service request number 606041153 Date service completed 29 May 2013

Agilent signature [Signature] Customer signature [Signature]

Total number of pages in this document 9 pages

Document Name:

Operator's training certificate and qualifications



## Certificate of Completion

Learner Name:

Saenguthai Tarak

Title Of Course:

ANCE-GCMS-2-041-D: 5977 EI/CI/HES MSD GC-MS OPER. H/W S/W – Intro, Repair and Troubleshooting

Completion Date:

March 18, 2016

Certified By Company:

Learning at Agilent

**All Service and Support training certificates have the following specific limitations.**

A certificate for Service and Support training is only valid while employed by Agilent Technologies or while working as an Agilent-authorized service provider, through which the service employee has ongoing access to Agilent's: Safety Alerts, Service Notes, internal technical updates, update training, current documentation, technical support, current parts, and parts updates. Completion of training alone, without being employed by Agilent Technologies, does not qualify an individual to safely install, service or maintain Agilent products.



Agilent Technologies

## Certificate of Completion

Learner Name:

Saenguthai Saeng Tarak

Title Of Course:

AN-CE-GC-II-022-A: Advanced GC Detectors Application and Troubleshooting Labs

Completion Date:

November 25, 2014

Certified By Company:

Learning at Agilent

**All Service and Support training certificates have the following specific limitations.**

A certificate for Service and Support training is only valid while employed by Agilent Technologies or while working as an Agilent-authorized service provider, through which the service employee has ongoing access to Agilent's: Safety Alerts, Service Notes, internal technical updates, update training, current documentation, technical support, current parts, and parts updates. Completion of training alone, without being employed by Agilent Technologies, does not qualify an individual to safely install, service or maintain Agilent products.

Date: September 6, 2018 6:11:18 PM

System ID: SGH545XYW

Page 37 / 38

## **BAROMETER**

**Equipment : Analog Barometer**

**ID No. / Tag No. : BM001/41**



MIRACLE INTERNATIONAL TECHNOLOGY CO., LTD.  
214 Bangwaek Rd. Bangrai Banglae Bangkok 10160  
Tel.: 0-2865-4647-8 Fax: 0-2865-4649 <http://www.mit.in.th>



ISO 9001:2015  
CALIBRATION 1002



## CALIBRATION CERTIFICATE

Certificate No.: L202405022-0013

Date Issued: 08-May-24

### Customer

: Eastern Thai Consulting 1992 Co., Ltd.  
683 Moo 11, Sukhapiarn 8 Rd., Nongkham, Sriracha, Chonburi 20230

### Equipment

: Analog Barometer

### Manufacturer

: Barigo

### Model

: -

### Serial No.

: -

### ID No./Tag No.

: BM001/41

### Date Received

: 03-May-24

### Date Calibrated

: 06-May-24

### Calibrated by

: Mr. Sanuth Srihukikul

### Calibration Method or Calibration Procedure Used

In-house method : CP-21 base on DKD-R 6-1: Edition 3 2014.

This certificate is traceable to national standards, which realize the units of measurement according to the International System of Units (SI).

### Result of Calibration

The reported uncertainty of measurement was based on standard uncertainty multiplied by a coverage factor  $k = 2$ , providing a level confidence approximately 95 percent.

This certificate may not be reproduced other than in full except with the prior written approval of the Miracle International Technology Company Limited.

Approved by:

*Saranyuth Tothua*  
(Mr. Saranyuth Tothua)

Page 1 of 2



COPY

Certificate No: L202405022-0013

Environment Ambient Temperature : (25 ± 2)°C

Relative Humidity : (50 ± 15)%RH

STD Reading	UUC Reading (mbar)	UUC Reading (mbar)	UUC Error	Uncertainty	MPE	Pass / Fail
mbar	Before Adjusted	After Adjusted	mbar	± mbar	± mbar	with Guard Band
990.00	990	-	0.00	0.59	10.3	Pass
1000.00	1000	-	0.00	0.59	10.3	Pass
1010.00	1010	-	0.00	0.59	10.3	Pass
1020.00	1020	-	0.00	0.59	10.3	Pass
1030.00	1030	-	0.00	0.59	10.3	Pass

STD = Standard Pass =  $|\text{error}| + |\text{uncertainty}| \leq |\text{MPE}|$

UUC = Unit Under Calibration Fail =  $|\text{error}| + |\text{uncertainty}| > |\text{MPE}|$

MPE = Maximum Permissible Error

Calibrated condition :

Pressure Medium Air : Density = 1.19 kg/m<sup>3</sup> @ 20°C, 1 bar  
Mounting Position Vertical  
Reference Level at center of its dial  
Conversion Factor Multiply by 1.0 E+02 - Pa unit

Description of UUC :

Range 930 - 1080 mbar Absolute  
Calibration Range 990 - 1030 mbar Absolute  
Scale Interval 1 mbar

Condition As-Received : Used Item

The measurement results and statements of conformity with specification only relate to the item calibrated.

Measurement Standards Used & Traceability :

The International System of Units (SI) through

iRPC Certificate No. CL1-P230097 for Reference Pressure Monitor Serial No. 1598, Due 09-Nov-24

End of Certificate

Page 2 of 2

COPY



**GAS CHROMATOGRAPH**

**Model : GC-2010 PLUS AF**

**Serial No. : C12095200986**

# SHIMADZU GAS CHROMATOGRAPH SYSTEM GC-2010Plus Series

## Operational Qualification

System Name		GC-2010Plus	
System ID No.		LNF 0413	
Installation Site		Tachikawa Research GC HC	

The undersigned performer reports that the Operational Qualification Protocol has been successfully completed for the system stated above.

Performer	Signature	Date
Print	Thirawat Rungtuan	15 / 02 / 2024
Title	Service Engineer	
Company	Proserv Scientific Co., Ltd	

The undersigned reviewer and manager report that the performer has completed the Operational Qualification Protocol successfully.

Reviewer	Signature	Date
Print	Panupong Bannong	15 / 02 / 2024
Title	Scientist	
Company	Environ Thins Consulting 1999 Co., Ltd	

Manager	Signature	Date
Print	Nunungat Bunkhantok	15 / 02 / 2024
Title	HS	
Company	Environ Thins Consulting 1999 Co., Ltd	

**COPY**

## Operational Qualification

## Operational Qualification Record

### 3. Operational Qualification Record

If the unit is included in the system to be inspected, place a checkmark in the "Applicable" box. If the unit is not included in the system, place a checkmark in the "Not Applicable" box. Enter a diagonal line in the Pass/Fail checkbox for "Not applicable" items.  
Here, inspection results are recorded along the procedure of Chapter 4 in Operational Qualification Protocol.

#### 3-1 Gas Chromatograph GC-2010Plus

Applicable ☒ Not Applicable ☐

Model Name										GC-2010Plus A.F.											
Component ID		LABE 04 / 3										C 1 2 0 9 5 2 0 0 7 2 C									
No.	Item	Criteria					Results					Pass	Fail								
1	Display, LED test	Verify the display and LED operation.	All LEDs light.	Screen contrast adjustment is possible.	LED Display								<input checked="" type="checkbox"/>	<input type="checkbox"/>							
		Verify the status and operation of all parts.	"Good" displayed as the result of the self-diagnostic test.										<input checked="" type="checkbox"/>	<input type="checkbox"/>							
2	Standard self-diagnostic test	Version number and build number are displayed.					Ver.					Version: 2.10200 Build No.: 20240					<input checked="" type="checkbox"/>	<input type="checkbox"/>			
3	Firmware version check	The version No. and build No. matches the controlled version number.					Controlled Ver. No.					Build No.: 2024					<input checked="" type="checkbox"/>	<input type="checkbox"/>			
4	Temperature test	Verify that temperature control is normal.	TEMP LED lights green.	Displayed actual values agree to the set values within ±1.0°C.	Temperature controller	(Name)	Set value	Measured value					<input checked="" type="checkbox"/>	<input type="checkbox"/>							
								COIL	50.0 °C	50.0 °C	50.0 °C										
								IN1	50.0 °C	50.0 °C	50.0 °C										
								IN2	50.0 °C	50.0 °C	50.0 °C										
								DET1	50.0 °C	50.0 °C	50.0 °C										
								DET2	50.0 °C	50.0 °C	50.0 °C										
								AUX3	50.0 °C	50.0 °C	50.0 °C										
								AUX4	50.0 °C	50.0 °C	50.0 °C										
								AUX5	50.0 °C	50.0 °C	50.0 °C										
								5	Column inlet pressure test	Verify the accuracy of the column inlet pressure.	Inspection pressure gauge reading 10.0kPa	Pressure gauge correction value			0.0 kPa					<input checked="" type="checkbox"/>	<input type="checkbox"/>
Pressure gauge reading	9.3 kPa																				
Post-correction reading	9.3 kPa																				
Pressure gauge correction value	0.4 kPa																				
Pressure gauge reading	1.97 kPa																				
5	Column inlet pressure test	Verify the accuracy of the column inlet pressure.	Inspection pressure gauge reading 200.0kPa	Pressure gauge correction value	0.3 kPa					<input checked="" type="checkbox"/>	<input type="checkbox"/>										
					Post-correction reading	1.97 kPa															
					Pressure gauge correction value	0.3 kPa															
					Pressure gauge reading	4.97 kPa															
					Post-correction reading	4.97 kPa															

Performer (signature): Thirawat Rungtuan Date: 15 / 02 / 2024

Reviewer (signature): Panupong Bannong Date: 15 / 02 / 2024

**COPY**

## Operational Qualification

## Operational Qualification Record

## Operational Qualification Record

No	Item	Criteria	Results	Pass	Fail
6	Pressure program test	Verify that the pressure program operates normally. Monitored pressure 6 minutes after start 250.0 ± 5.0 kPa	250.0 ± 5.0 kPa	<input checked="" type="checkbox"/>	<input type="checkbox"/>
7	Flowrate test	Verify the accuracy of the full-flow and septum purging. Septum purge vent measured flow rate 3.00 ± 0.10 mL/min Total of septum purge and split vent flow rate values 10.00 ± 3.00 mL/min	Septum purge 3.00 mL/min Split vent 1.00 mL/min Total 4.00 mL/min	<input checked="" type="checkbox"/>	<input type="checkbox"/>
8	Column oven test	Verify the accuracy of the column oven temperature. Total of septum purge and split vent flow rate values 300.2 ± 20.0 mL/min (Carrier gas: N <sub>2</sub> ) Total of septum purge and split vent flow rate values 500.2 ± 35.0 mL/min (Carrier gas: He)	Temp. correction value Temp. sensor reading 52.0 °C Corrected temp. value 51.6 °C Inspection Temp. sensor reading 150.0 ± 4.2 °C Corrected temp. value 150.0 ± 4.2 °C Inspection Temp. sensor reading 280.0 ± 5.5 °C Corrected temp. value 280.0 ± 5.5 °C	<input checked="" type="checkbox"/>	<input type="checkbox"/>
9	Temperature program test	Verify that the temperature program operates normally. Monitored temperature 6 minutes after start 200 ± 1 °C Inspection temperature reading 8 minutes after start 200.0 ± 4.7 °C Using a temperature sensor with 1 °C minimum display increment 200.43 °C	90.0 °C 200.0 ± 4.7 °C 200.43 °C	<input checked="" type="checkbox"/>	<input type="checkbox"/>
10	Sensitivity test	Verify the detector sensitivity. FID <input checked="" type="checkbox"/> Applicable <input type="checkbox"/> Not Applicable Calculated S value 10.0 × 10 <sup>3</sup> C/g min. Make-up gas: N <sub>2</sub> 7.00 × 10 <sup>3</sup> C/g min. TCD <input type="checkbox"/> Applicable <input checked="" type="checkbox"/> Not Applicable Calculated S value 4.00 × 10 <sup>3</sup> mV/mg min.	C <sub>10</sub> AREA value 47787 Calculated S value 15.30 × 10 <sup>3</sup> C/g C <sub>10</sub> AREA value Flowrate at vent Calculated S value	<input checked="" type="checkbox"/>	<input type="checkbox"/>

Performer (signature): Om Date: 15 / 08 / 2024  
Reviewer (signature): Om Date: 15 / 08 / 2024

COPY

## 3-2 AOC-20i Auto Injector

☒ Applicable ☐ Not Applicable☒ Single ☐ Dual system, main injector

Component ID		Model Name	AOC-20i
Serial No. (S/N)		C 1 2 1 2 5 4 1 0 3 0 9	
No.	Item	Criteria	Results
1	Display, LED test	Verify the display and LED operation. All LEDs light, except decimal point.	<input checked="" type="checkbox"/>
2	ROM, RAM self diagnosis	Verify that ROM and RAM memory operates normally. Display shows "000".	<input checked="" type="checkbox"/>
3	Firmware version check	Verify the version number is displayed. The version number matches the controlled version number.	3.4
4	Basic operation test	Verify that the auto injector basic operation is correct. Sample injected into the GC and GC operation starts.	3.4

☒ Not Applicable ☐ Dual system, sub injector

Component ID		Model Name	AOC-20i
Serial No. (S/N)			
No.	Item	Criteria	Results
1	Display, LED test	Verify the display and LED operation. All LEDs light, except decimal point.	<input type="checkbox"/>
2	ROM, RAM self diagnosis	Verify that ROM and RAM memory operates normally. Display shows "000".	<input type="checkbox"/>
3	Firmware version check	Verify the version number is displayed. The version number matches the controlled version number.	<input type="checkbox"/>
4	Basic operation test	Verify that the auto injector basic operation is correct. Sample No. 1 transferred to the main injector, sample No. 2 transferred to the sub-injector. Sub-injector injects into the GC simultaneously with the main AOC.	<input type="checkbox"/>

Performer (signature): Om Date: 15 / 08 / 2024  
Reviewer (signature): Om Date: 15 / 08 / 2024

COPY

## Operational Qualification Operational Qualification Record

## 3-3 AOC-20s Auto Sampler

☒ Applicable ☐ Not Applicable

Component ID		Model Name		AOC-20s	
Serial No. (SN)		L P 0 E Q 1 7		C 1 2 1 3 5 4 0 5 6 1 0	
No.	Item	Criteria	Results	Pass	Fail
1	Initial operation test	Verify that the auto sampler basic operation is correct.	LED lights green, run red.	<input checked="" type="checkbox"/>	<input type="checkbox"/>
2	Firmware version check	Verify the program version. The version number is displayed. The version number matches the controlled version number.	Version No. 3.5 Controlled Ver. No. 3.5	<input checked="" type="checkbox"/>	<input type="checkbox"/>

Performer (signature):

Date: 15 / 03 / 2024

Reviewer (signature):

Date: 15 / 03 / 2024

## Operational Qualification

## Operational Qualification Record

## 3-4 SPL-2010Plus Split/Splitless Injection Unit

☒ Applicable ☐ Not Applicable

Component ID		Model Name		SPL-2010Plus	
Serial No. (SN)					
No.	Item	Criteria	Results	Pass	Fail
1	Column inlet pressure test	Verify the accuracy of the column inlet pressure. Inspection pressure gauge reading $\square 10.0 \pm 3.0 \text{ kPa}$ Inspection pressure gauge reading $\square 200.0 \pm 20.0 \text{ kPa}$ Inspection pressure gauge reading $\square 500.0 \pm 50.0 \text{ kPa}$	Pressure gauge correction value Pressure gauge reading kPa Post-correction reading kPa Pressure gauge correction value kPa Pressure gauge reading kPa Post-correction reading kPa Pressure gauge correction value kPa Pressure gauge reading kPa Post-correction reading kPa	<input type="checkbox"/>	<input type="checkbox"/>
2	Pressure program test	Verify that the pressure program operates normally. Monitored pressure 6 minutes after start $250.0 \pm 5.0 \text{ kPa}$ Inspection pressure gauge reading 8 minutes after start $250.0 \pm 20.0 \text{ kPa}$	Pressure gauge correction value Pressure gauge reading kPa Post-correction reading kPa	<input type="checkbox"/>	<input type="checkbox"/>
3	Flowrate test	Verify the accuracy of the full-flow and septum purging. Septum purge vent measured flow rate $3.0 \pm 1.0 \text{ mL/min}$ Total of septum purge and split vent flow rate values $10.0 \pm 3.0 \text{ mL/min}$ Total of septum purge and split vent flow rate values $200.0 \pm 20.0 \text{ mL/min}$ Total of septum purge and split vent flow rate values $300.0 \pm 30.0 \text{ mL/min}$ Total of septum purge and split vent flow rate values $500.0 \pm 50.0 \text{ mL/min}$	Septum purge mL/min Split vent mL/min Total mL/min Split vent mL/min Total mL/min Split vent mL/min Total mL/min	<input type="checkbox"/>	<input type="checkbox"/>

Performer (signature):

Date: 15 / 03 / 2024

Reviewer (signature):

Date: 15 / 03 / 2024

**Primary Flow Calibrator**

**Serial No. : 110619 , 207510**





# CALIBRATION LABORATORY CO., LTD.

2/10-11, 14, 55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd, Ladphrao, Bangkok 10230  
Tel: 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail: sale@cal-laboratory.com



# CALIBRATION LABORATORY CO., LTD.

2/10-11, 14, 55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd, Ladphrao, Bangkok 10230  
Tel: 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail: sale@cal-laboratory.com



## CERTIFICATE OF CALIBRATION

### FOR

NOMENCLATURE : FLOW METER  
MANUFACTURER : BIOS INTERNATIONAL  
MODEL / TYPE : DEFENDER 510-L  
SERIAL NO. : 110619  
CLID. NO. : 212500238  
JOB CONTROL NO. : 250128010260  
CALIBRATION SERVICE : ☒ IN-LABORATORY ☐ ON-SITE

CUSTOMER : EASTERN THAI CONSULTING 1992 CO., LTD.  
683 MOO 11, SUKHAPIBARN 8 RD,  
NONGKHAM, SRIRACHA, CHONBURI 20230

DATE OF RECEIVED : 28 January 2025

DATE OF ISSUED : 31 January 2025

The report of calibration shall not be reproduced except in full without approval of the Calibration Laboratory Co., Ltd.

Calibrated By : Supphakit Sakuntaharn  
Calibration Engineer



Approved By : Mongkol Yotsoontorn  
Authorized Signatory  
31 January 2025

This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to the International System of Units (SI)

Certificate No. Q25010260  
F3-011-05/12-23



page 1 of 3  
electcalibration

## REPORT OF CALIBRATION

### FOR

NOMENCLATURE : FLOW METER  
MANUFACTURER : BIOS INTERNATIONAL  
MODEL / TYPE : DEFENDER 510-L  
SERIAL NO. : 110619  
DATE OF CALIBRATION : 29 January 2025

#### ENVIRONMENT CONDITIONS :

Temperature :  $(23 \pm 2) ^\circ\text{C}$  Relative Humidity :  $(55 \pm 10) \% \text{ RH}$

#### PROCEDURE USED :

This instrument was calibrated under procedure No. CLC-CPPF-03. The calibration was performed by comparison with Gas Flow Meter which refers to the standard condition of  $101.325 \text{ kPa}$  and  $0 ^\circ\text{C}$ .

#### REFERENCE STANDARD USED :

Gas Flow Meter, Alicat Scientific Model M-500SCCM-D-DB15 S/N. 261329.

#### TRACEABILITY :


The measurements are traceable to International System of Units (SI), through Chell Instrument Ltd. Certificate No. N037063, Due Date 26 February 2025.

#### UNCERTAINTY :

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor complies with the table which for a normal distribution corresponds to a coverage probability of approximately 95 %.

It has been evaluated according to the "Evaluation of the Uncertainty of Measurement in Calibration (EA-4/02 M:2022)"

Certificate No. Q25010260  
F3-011-05/12-23



page 2 of 3  
electcalibration







# CALIBRATION LABORATORY CO., LTD.

210-114, 55 Soi Prasert Manukul 29 Yek 4 Prasert Manukul Rd. 1 addhrai, Bangkok 10230  
Tel: 02-578-0353-4 Fax: 02-578-2672 www.calibration.co.th E-mail: sale@calibration.co.th



CLC  
Accredited  
ISO/IEC 17025

CONDITION OF CALIBRATION ITEM : RECEIVED IN GOOD OPERATIONAL CONDITION

MEASUREMENT RESULTS : ( X ) without adjustment ( ) adjustment

The table in the following gives the calibration results and associated measurement uncertainties of the measuring flow meter.

## CALIBRATION DATA

### FLOW METER RESULT

Nominal Value ( cc/min )	STD Applied ( cc/min )	DUC Reading ( cc/min )	Correction ( cc/min )	Uncertainty $\pm$ ( cc/min )
0	0.00	0.00	0.00	-
50	50.00	48.75	+1.25	2.10
100	100.00	97.66	+2.34	2.10
200	200.00	195.22	+4.78	2.10
300	300.00	292.56	+7.44	2.10
400	400.00	390.82	+9.18	2.10
500	500.00	490.04	+9.96	2.10

Technical Note, Media of Gas : Air

Setting Temperature 0 ° C ; Pressure 101.3 kPa

Note. The Scope of Accredited ANAB Certificate No. ACDM-2814 Version 014 Page 49 of 68

This report is valid for the above stated instrument/s only.

### End of Certificate ###

Certificate No. Q25010260

F3-011-05/12-23



page 3 of 3



# CALIBRATION LABORATORY CO., LTD.

2/10-11 14, 55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd, Ladphrao, Bangkok 10230  
Tel 02-578-0353-4 Fax 02-578-2672 www.cal-laboratory.com E-mail: sale@cal-laboratory.com



ANAB  
Accredited  
ISO/IEC 17025



## CERTIFICATE OF CALIBRATION

### FOR

NOMENCLATURE : FLOW METER  
MANUFACTURER : MESALABS  
MODEL / TYPE : DEFENDER 510-M  
SERIAL NO. : 207510  
CLID. NO. : 212500237  
JOB CONTROL NO. : 250128010259  
CALIBRATION SERVICE : ☒ IN-LABORATORY ☐ ON-SITE

CUSTOMER : EASTERN THAI CONSULTING 1992 CO., LTD.  
683 MOO 11, SUKHAPIBARN 8 RD,  
NONGKHAM, SRIRACHA, CHONBURI 20230


DATE OF RECEIVED : 28 January 2025

DATE OF ISSUED : 31 January 2025

The report of calibration shall not be reproduced except in full without approval of the Calibration Laboratory Co., Ltd.

Calibrated By :

Suphakit Sakuntaharn  
Calibration Engineer



Approved By :


Mongkol Yotsoontorn  
Authorized Signatory

31 January 2025

This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to the International System of Units (SI)

Certificate No. Q25010259

F3-011-05/12-23



# CALIBRATION LABORATORY CO., LTD.

2/10-11 14, 55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd, Ladphrao, Bangkok 10230  
Tel 02-578-0353-4 Fax 02-578-2672 www.cal-laboratory.com E-mail: sale@cal-laboratory.com



ANAB  
Accredited  
ISO/IEC 17025

## REPORT OF CALIBRATION

### FOR

NOMENCLATURE : FLOW METER  
MANUFACTURER : MESALABS  
MODEL / TYPE : DEFENDER 510-M  
SERIAL NO. : 207510  
DATE OF CALIBRATION : 29 January 2025

#### ENVIRONMENT CONDITIONS :

Temperature :  $(23 \pm 2) ^\circ\text{C}$  Relative Humidity :  $(55 \pm 10) \% \text{ RH}$

#### PROCEDURE USED :

This instrument was calibrated under procedure No. CLC-CPPF-03. The calibration was performed by comparison with Gas Flow Meter which refers to the standard condition of 101.325 kPa and 0  $^\circ\text{C}$ .

#### REFERENCE STANDARD USED :

Gas Flow Meter, Alicat Scientific Model M-500SCCM-D-DB15 S/N. 261329.

#### TRACEABILITY :

The measurements are traceable to International System of Units (SI), through Chell Instrument Ltd.  
Certificate No. N037063, Due Date 26 February 2025.

#### UNCERTAINTY :

The reported expanded uncertainty of measurement is stated as the standard uncertainty multiplied by the coverage factor complies with the table which for a normal distribution corresponds to a coverage probability of approximately 95 %.  
It has been evaluated according to the "Evaluation of the Uncertainty of Measurement in Calibration (EA-4/02 M:2022)"

Certificate No. Q25010259

F3-011-05/12-23





# CALIBRATION LABORATORY CO., LTD.

210-11, 14, 35 Soi Prasert Manukul 29 Yaek 4, Prasert Manukul Rd., Ladphrao Bangkok 10230  
Tel: 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail: sale@cal-laboratory.com



CONDITION OF CALIBRATION ITEM : RECEIVED IN GOOD OPERATIONAL CONDITION

MEASUREMENT RESULTS : ( X ) without adjustment ( ) adjustment

The table in the following gives the calibration results and associated measurement uncertainties of the measuring flow meter.

## CALIBRATION DATA

### FLOW METER RESULT

Nominal Value ( cc/min )	STD Applied ( cc/min )	DUC Reading ( cc/min )	Correction ( cc/min )	Uncertainty $\pm$ ( cc/min )
0	0.00	0.00	0.00	
50	50.00	45.81	+4.19	2.10
100	100.00	99.10	+0.90	2.10
200	200.00	198.03	+1.97	2.10
300	300.00	298.30	+1.70	2.10
400	400.00	396.50	+3.50	2.10
500	500.00	495.31	+4.69	2.10

Technical Note Media of Gas : Air

Setting Temperature 0 ° C ; Pressure 101.3 kPa

Note. The Scope of Accredited ANAB Certificate No. ACDM-2814 Version 014 Page 49 of 68

This report is valid for the above stated instrument/s only.

### End of Certificate ###

Certificate No. Q25010259  
F3-011-05/12-23



page 3 of 3

ภาคผนวก ช

---

ใบรับรองความสามารถห้องปฏิบัติการ



แบบ กมช./สมอ.๒  
Form NSC/TISI 2

ใบรับรองเลขที่ 23-LB0251  
(Certificate No.)

## ใบรับรองระบบงาน (Certificate of Accreditation)

อาศัยอำนาจตามความในพระราชบัญญัติการมาตรฐานแห่งชาติ พ.ศ. ๒๕๕๑  
(By Virtue of National Standardization Act B.E. 2551 (2008))

เลขาธิการสำนักงานมาตรฐานผลิตภัณฑ์อุตสาหกรรม  
(Secretary-General, Thai Industrial Standards Institute)

ออกใบรับรองฉบับนี้ให้  
(Issues this certificate to)

บริษัท อีสเทิร์น ไทย คอนซัลติ้ง 1992 จำกัด  
(Eastern Thai Consulting 1992 Co., Ltd.)

ตั้งอยู่เลขที่  
(Address)

๖๘๓ หมู่ที่ ๑๑ ถนนสุขาภิบาล ๘ ตำบลหนองขาม อำเภอสรีราชา จังหวัดชลบุรี  
(683 Moo 11, Sukhapibarn 8 Road, Nongkham, Sriracha, Chonburi)

ได้รับการรับรองความสามารถ  
(Certificate of competence)

ตามมาตรฐานเลขที่ มอก. ๑๗๐๒๕ - ๒๕๖๑  
(Standard No. TIS 17025-2561 (2018) (ISO/IEC 17025: 2017))

ข้อกำหนดทั่วไปว่าด้วยความสามารถของ ห้องปฏิบัติการทดสอบและห้องปฏิบัติการสอบเทียบ  
(General requirements for the competence of testing and calibration laboratories)

หมายเลขการรับรองที่ ทดสอบ ๑๗๑๒  
(Accreditation No. Testing 1712)

โดยมีรายละเอียดสาขาและขอบข่ายที่ได้ใบรับรอง แสดงไว้ใน QR CODE และ [www.tisi.go.th](http://www.tisi.go.th)  
(Details of the scheme and scope of the certificate are shown in QR CODE and [www.tisi.go.th](http://www.tisi.go.th))

ออกให้ ณ วันที่ ๒๓ สิงหาคม พ.ศ. ๒๕๖๖  
(Issue date : 23 August B.E. 2566 (2023))

(นายเอกนิติ รมยานนท์)

รองเลขาธิการสำนักงานมาตรฐานผลิตภัณฑ์อุตสาหกรรม

ปฏิบัติราชการแทน

เลขาธิการสำนักงานมาตรฐานผลิตภัณฑ์อุตสาหกรรม



กระทรวงอุตสาหกรรม สำนักงานมาตรฐานผลิตภัณฑ์อุตสาหกรรม  
(Ministry of Industry Thailand, Thai Industrial Standards Institute)



รายละเอียดสาขาและขอบข่ายใบรับรองห้องปฏิบัติการ  
(Scope of Accreditation for Testing)  
ใบรับรองเลขที่ 23-LB0251  
(Certification No. 23-LB0251)



ชื่อห้องปฏิบัติการ  
(Laboratory Name)

บริษัท อีสเทิร์น ไทย คอนซัลติ้ง 1992 จำกัด  
(Eastern Thai Consulting 1992 Co., Ltd.)

หมายเลขการรับรองที่  
(Accreditation No.)

ทดสอบ 1712  
(Testing 1712)

ฉบับที่ 01  
(Issue No.01)

ออกให้ตั้งแต่วันที่ 17 กรกฎาคม พ.ศ. 2566  
(Valid from) (17 July B.E.2566 (2023))

ถึงวันที่ 16 กรกฎาคม พ.ศ. 2571  
(Until) (16 July B.E.2571 (2028))

สถานภาพห้องปฏิบัติการ  
(Laboratory status)

☒ ถาวร  
(Permanent)

☐ นอกสถานที่  
(Site)

☐ชั่วคราว  
(Temporary)

☐เคลื่อนที่  
(Mobile)

☐หลายสถานที่  
(Multisite)

สาขาการทดสอบ (Field of Testing)	รายการทดสอบ (Parameter)	วิธีทดสอบ (Test Method)
สาขาสังแวดล้อม (Environmental field) 1. น้ำ ( Water )	- โลหะหนัก (Heavy metal) • โครเมียม (Cr) 0.03 mg/L to 2.00 mg/L • ทองแดง (Cu) 0.03 mg/L to 2.00 mg/L • เหล็ก (Fe) 0.03 mg/L to 2.00 mg/L • ตะกั่ว (Pb) 0.01 mg/L to 1.00 mg/L • นิกเกิล (Ni) 0.03 mg/L to 2.00 mg/L • อลูมิเนียม (Al) 0.10 mg/L to 2.00 mg/L • แบเรียม (Ba) 0.03 mg/L to 2.00 mg/L • แคดเมียม (Cd) 0.003 mg/L to 1.00 mg/L • แมงกานีส (Mn) 0.03 mg/L to 2.00 mg/L • เงิน (Ag) 0.05 mg/L to 2.00 mg/L • สังกะสี (Zn) 0.03 mg/L to 2.00 mg/L	- Standard Method for the Examination of Water and Wastewater, APHA, AWWA, WEF 23 <sup>rd</sup> edition 2017. Part 3030 F and 3120 B 

กระทรวงอุตสาหกรรม สำนักงานมาตรฐานผลิตภัณฑ์อุตสาหกรรม  
(Ministry of Industry, Thai Industrial Standards Institute)

หน้าที่ 1/5

รายละเอียดสาขาและขอบข่ายใบรับรองห้องปฏิบัติการ

(Scope of Accreditation for Testing)

ใบรับรองเลขที่ 23-LB0251

(Certification No. 23-LB0251)



ฉบับที่ 01  
(Issue No.)

ออกให้ตั้งแต่วันที่ 17 กรกฎาคม พ.ศ. 2566  
(Valid from) (17 July B.E.2566 (2023))

ถึงวันที่ 16 กรกฎาคม พ.ศ. 2571  
(Until) (16 July B.E.2571 (2028))

สถานภาพห้องปฏิบัติการ  
(Laboratory status)

☒ ถาวร  
(Permanent)

☐ นอกสถานที่  
(Site)

☐ชั่วคราว  
(Temporary)

☐เคลื่อนที่  
(Mobile)

☐หลายสถานที่  
(Multisite)

สาขาการทดสอบ (Field of Testing)	รายการทดสอบ (Parameter)	วิธีทดสอบ (Test Method)
<p>สาขาสังแวดล้อม (Environmental field)</p> <p>1. น้ำ (ต่อ) (Water ) (cont.)</p>	<p>- ไขมันและน้ำมัน (Oil &amp; Grease) 3.0 mg/L - 20.0 mg/L</p>	<p>- Standard Method for the Examination of Water and Wastewater, APHA, AWWA, WEF 23<sup>rd</sup> edition 2017. Part 5520 B</p>
<p>2. น้ำเสีย (Wastewater )</p>	<p>- โลหะหนัก (Heavy metal)</p> <ul style="list-style-type: none"> <li>โครเมียม (Cr) 0.03 mg/L to 2.00 mg/L</li> <li>ทองแดง (Cu) 0.03 mg/L to 2.00 mg/L</li> <li>เหล็ก (Fe) 0.03 mg/L to 2.00 mg/L</li> <li>ตะกั่ว (Pb) 0.03 mg/L to 2.00 mg/L</li> <li>นิกเกิล (Ni) 0.03 mg/L to 2.00 mg/L</li> <li>อลูมิเนียม (Al) 0.10 mg/L to 2.00 mg/L</li> <li>แบเรียม (Ba) 0.03 mg/L to 2.00 mg/L</li> <li>แคดเมียม (Cd) 0.03 mg/L to 2.00 mg/L</li> </ul>	<p>- Standard Method for the Examination of Water and Wastewater, APHA, AWWA, WEF 23<sup>rd</sup> edition 2017. Part 3030 F and 3120 B</p>

รายละเอียดสาขาและขอบข่ายใบรับรองห้องปฏิบัติการ

(Scope of Accreditation for Testing)

ใบรับรองเลขที่ 23-LB0251

(Certification No. 23-LB0251)



ฉบับที่ 01  
(Issue No.01)

ออกให้ตั้งแต่วันที่ 17 กรกฎาคม พ.ศ. 2566  
(Valid from) (17 July B.E.2566 (2023))

ถึงวันที่ 16 กรกฎาคม พ.ศ. 2571  
(Until) (16 July B.E.2571 (2028))

สถานภาพห้องปฏิบัติการ  
(Laboratory status)

☒ ถาวร  
(Permanent)

☐นอกสถานที่  
(Site)

☐ชั่วคราว  
(Temporary)

☐เคลื่อนที่  
(Mobile)

☐หลายสถานที่  
(Multisite)

สาขาการทดสอบ (Field of Testing)	รายการทดสอบ (Parameter)	วิธีทดสอบ (Test Method)
<p>สาขาสังแวดล้อม (Environmental field)</p> <p>2. น้ำเสีย (ต่อ) (Wastewater ) (cont.)</p>	<p>- โลหะหนัก (ต่อ) (Heavy metal) (cont.)</p> <ul style="list-style-type: none"> <li>แมงกานีส (Mn) 0.03 mg/L to 2.00 mg/L</li> <li>เงิน (Ag) 0.05 mg/L to 2.00 mg/L</li> <li>สังกะสี (Zn) 0.03 mg/L to 2.00 mg/L</li> </ul> <p>- ไขมันและน้ำมัน (Oil &amp; Grease) 3.0 mg/L - 20.0 mg/L</p>	<p>- Standard Method for the Examination of Water and Wastewater, APHA, AWWA, WEF 23<sup>rd</sup> edition 2017. Part 3030 F and 3120 B</p> <p>- Standard Method for the Examination of Water and Wastewater, APHA, AWWA, WEF 23<sup>rd</sup> edition 2017. Part 5520 B</p>



รายละเอียดสาขาและขอบข่ายใบรับรองห้องปฏิบัติการ

(Scope of Accreditation for Testing)

ใบรับรองเลขที่ 23-LB0251

(Certification No. 23-LB0251)



ฉบับที่ 01  
(Issue No.)

ออกให้ตั้งแต่วันที่ 17 กรกฎาคม พ.ศ. 2566  
(Valid from) (17 July B.E.2566 (2023))

ถึงวันที่ 16 กรกฎาคม พ.ศ. 2571  
(Until) (16 July B.E.2571 (2028))

สถานภาพห้องปฏิบัติการ  
(Laboratory status)

☐ ถาวร  
(Permanent)

☒ นอกสถานที่  
(Site)

☐ชั่วคราว  
(Temporary)

☐เคลื่อนที่  
(Mobile)

☐หลายสถานที่  
(Multisite)

สาขาการทดสอบ (Field of Testing)	รายการทดสอบ (Parameter)	วิธีทดสอบ (Test Method)
<p>สาขาสังแวดล้อม (Environmental field)</p> <p>3.พื้นที่การทำงาน (Workplace)</p>	<p>- ระดับเสียง (Sound Level)</p> <ul style="list-style-type: none"> <li>ระดับเสียงเฉลี่ย <math>L_{eqT}</math> ช่วง 30 - 130 dB(A)</li> <li>ระดับเสียงสูงสุด <math>L_{max}</math> ช่วง 30 - 130 dB(A)</li> </ul>	<p>- ISO 11202:2010</p> <p>- ประกาศกระทรวงอุตสาหกรรม เรื่องมาตรการคุ้มครองความปลอดภัยในการประกอบกิจการโรงงานเกี่ยวกับสภาวะแวดล้อมในการทำงาน พ.ศ.2546 ลงวันที่ 6 พ.ย. 2546 (Notification of The Ministry of Industry B.E. 2546 (2003) on the Safety Protection Measures in Factory Regarding Working Area Environment, dated November 6, 2003)</p> <p>- ประกาศกรมสวัสดิการและคุ้มครองแรงงาน เรื่องมาตรฐานระดับเสียงที่ยอมให้ลูกจ้างได้รับเฉลี่ยตลอดระยะเวลาการทำงานในแต่ละวัน ลงวันที่ 13 ธ.ค. 2560 (Notification of the Department of Labor Protection and Welfare on the standard of noise level that employees are allowed to receive in average period of work each day, dated December 13, 2017.)</p> <p>- ประกาศกรมสวัสดิการและคุ้มครองแรงงาน เรื่องหลักเกณฑ์ วิธีการตรวจวัดและการวิเคราะห์สภาวะการทำงานเกี่ยวกับระดับความร้อน แสงสว่าง หรือเสียง รวมทั้งระยะเวลาและประเภทกิจการที่ต้องดำเนินการ ลงวันที่ 8 ก.พ. 2561 (Notification of the Department of Labor Protection and Welfare on Criteria, Measurement Methods, and Analysis of Working Conditions Regarding Heat, Light, or Noise Levels, Including Duration and Types of Businesses to Be Performed, dated February 8, 2018.)</p>

กระทรวงอุตสาหกรรมสำนักงานมาตรฐานผลิตภัณฑ์อุตสาหกรรม  
(Ministry of Industry, Thai Industrial Standards Institute)

หน้าที่ 4/5

รายละเอียดสาขาและขอบข่ายใบรับรองห้องปฏิบัติการ

(Scope of Accreditation for Testing)

ใบรับรองเลขที่ 23-LB0251

(Certification No. 23-LB0251)



ฉบับที่ 01  
(Issue No.)

ออกให้ตั้งแต่วันที่ 17 กรกฎาคม พ.ศ. 2566  
(Valid from) (17 July B.E.2566 (2023))

ถึงวันที่ 16 กรกฎาคม พ.ศ. 2571  
(Until) (16 July B.E.2571 (2028))

สถานภาพห้องปฏิบัติการ  
(Laboratory status)

☐ ถาวร  
(Permanent)

☒นอกสถานที่  
(Site)

☐ชั่วคราว  
(Temporary)

☐เคลื่อนที่  
(Mobile)

☐หลายสถานที่  
(Multisite)

สาขาการทดสอบ (Field of Testing)	รายการทดสอบ (Parameter)	วิธีทดสอบ (Test Method)
<p>สาขาสังแวดล้อม (Environmental field)</p> <p>4. บรรยากาศ (Ambient)</p>	<p>- ระดับเสียง (Sound Level)</p> <ul style="list-style-type: none"> <li>ระดับเสียงเฉลี่ย <math>L_{eqT}</math> ช่วง 30.0 - 130.0 dB(A)</li> <li>ระดับเสียงสูงสุด <math>L_{max}</math> ช่วง 30.0 - 130.0 dB(A)</li> </ul>	<p>- ISO 1996 - 1 : 2016</p> <p>- ประกาศคณะกรรมการสิ่งแวดล้อมแห่งชาติ ฉบับที่ 15 (2540) เรื่องกำหนด มาตรฐานระดับเสียงโดยทั่วไป ลงวันที่ 12 มี.ค. 2540 (Notification of The National Environmental Board Volume 15 B.E. 2540 (1997) on the general noise level standards, dated March 12, 1997)</p> <p>- ประกาศกรมควบคุมมลพิษ เรื่อง การคำนวณค่าระดับเสียง ลงวันที่ 11 ส.ค. 2540 (Notification of the Pollution Control Department on the calculation of the noise level, dated August 11, 1997.)</p> <p>- ประกาศกรมโรงงานอุตสาหกรรม เรื่องวิธีการตรวจวัดระดับเสียงการรบกวน ระดับเสียงเฉลี่ย 24 ชั่วโมง และระดับเสียงสูงสุดที่เกิดจากการประกอบกิจการโรงงาน พ.ศ. 2553 ลงวันที่ 20 ธ.ค. 2553 (Notification of the Department of Industrial Works on Methods for Measuring Noise Annoyance, Noise Levels 24-Hour Average and Maximum Noise Level from Factory B.E. 2553, dated December 20, 2010.)</p>

กระทรวงอุตสาหกรรมสำนักงานมาตรฐานผลิตภัณฑ์อุตสาหกรรม  
(Ministry of Industry, Thai Industrial Standards Institute)

หน้าที่ 5/5



ที่ อว 0303/18183

## ใบรับรองความสามารถห้องปฏิบัติการทดสอบ

ใบรับรองฉบับนี้ให้ไว้เพื่อแสดงว่า

ห้องปฏิบัติการ บริษัท อีสเทิร์น ไทย คอนซัลตติ้ง 1992 จำกัด  
เลขที่ 683 หมู่ที่ 11 ถนนสุขุมวิท 8 ตำบลหนองขาม  
อำเภอศรีราชา จังหวัดชลบุรี 20230

ได้ผ่านการประเมินความสามารถห้องปฏิบัติการทดสอบตามมาตรฐาน ISO/IEC 17025 : 2017  
และข้อกำหนด กฎระเบียบ และเงื่อนไขการรับรองความสามารถห้องปฏิบัติการทดสอบ  
ของกองบริหารและรับรองห้องปฏิบัติการ กรมวิทยาศาสตร์บริการ

หมายเลขการรับรองระบบงานที่ ทดสอบ - 0159

รายละเอียดการรับรองดังขอข่ายการรับรองแนบท้าย

ออกให้ ณ วันที่ : 7 พฤศจิกายน 2566

หมดอายุ วันที่ : 6 พฤศจิกายน 2570

ลงชื่อ : 

(นางจันทร์นวี วรสรรพวิทย์)

นักวิทยาศาสตร์ชำนาญการพิเศษ

รักษาราชการแทน ผู้อำนวยการกองบริหารและรับรองห้องปฏิบัติการ

กองบริหารและรับรองห้องปฏิบัติการ กรมวิทยาศาสตร์บริการ  
กระทรวงการอุดมศึกษา วิทยาศาสตร์ วิจัย และนวัตกรรม

ที่ อว 0303/18183

## ขอข่ายการรับรองความสามารถห้องปฏิบัติการทดสอบ

ชื่อห้องปฏิบัติการ : ห้องปฏิบัติการ บริษัท อีสเทิร์น ไทย คอนซัลตติ้ง 1992 จำกัด

สถานที่ตั้ง : เลขที่ 683 หมู่ที่ 11 ถนนสุขุมวิท 8 ตำบลหนองขาม

อำเภอศรีราชา จังหวัดชลบุรี 20230

หมายเลขการรับรองระบบงานที่ : ทดสอบ - 0159

สถานะของห้องปฏิบัติการ : ☒ ถาวร ☐ นอกสถานที่ ☐ชั่วคราว ☐เคลื่อนที่

ลำดับ ที่	วัสดุ / ผลิตภัณฑ์ที่ทดสอบ	รายการที่ทดสอบ / ช่วงของการทดสอบ	วิธีทดสอบ / เทคนิคที่ใช้
1	น้ำ	- ซีโอดี 40 mg/L ถึง 5 000 mg/L  - โปรท 0.001 mg/L ถึง 0.02 mg/L  - บีโอดี 2 mg/L ถึง 5 000 mg/L	Standard Methods for the Examination of Water and Wastewater, APHA, AWWA & WEF, 23 <sup>rd</sup> ed., 2017, part 5220 C  Standard Methods for the Examination of Water and Wastewater, APHA, AWWA & WEF, 23 <sup>rd</sup> ed., 2017, part 3112 B  Standard Methods for the Examination of Water and Wastewater, APHA, AWWA & WEF, 23 <sup>rd</sup> ed., 2017, part 5210 B

ออกครั้งแรก ณ วันที่ 21 พฤศจิกายน 2560

ฉบับที่ 4

กองบริหารและรับรองห้องปฏิบัติการ กรมวิทยาศาสตร์บริการ กระทรวงการอุดมศึกษา วิทยาศาสตร์ วิจัย และนวัตกรรม

## ขอข่ายการรับรองความสามารถห้องปฏิบัติการทดสอบ

ชื่อห้องปฏิบัติการ : ห้องปฏิบัติการ บริษัท อีสเทิร์น ไทย คอนซัลต์ติ้ง 1992 จำกัด  
 สถานที่ตั้ง : เลขที่ 683 หมู่ที่ 11 ถนนสุขาภิบาล 8 ตำบลหนองขาม  
 อำเภอสรีราชา จังหวัดชลบุรี 20230

หมายเลขการรับรองระบบงานที่ : ทดสอบ - 0159

สถานะของห้องปฏิบัติการ : ☒ ถาวร ☐ นอกสถานที่ ☐ชั่วคราว ☐เคลื่อนที่

ลำดับ ที่	วัสดุ / ผลิตภัณฑ์ที่ทดสอบ	รายการที่ทดสอบ / ช่วงของการทดสอบ	วิธีทดสอบ / เทคนิคที่ใช้
1 (ต่อ)	น้ำ	- สารที่ละลายได้ทั้งหมด ที่อุณหภูมิ 180 °C 25 mg/L ถึง 10 000 mg/L  - สารแขวนลอยทั้งหมด ที่อุณหภูมิ 103 °C ถึง 105 °C 5 mg/L ถึง 2 000 mg/L  - ฟลูออไรด์ 0.5 mg/L ถึง 10 mg/L	Standard Methods for the Examination of Water and Wastewater, APHA, AWWA & WEF, 23 <sup>rd</sup> ed., 2017, part 2540 C  Standard Methods for the Examination of Water and Wastewater, APHA, AWWA & WEF, 23 <sup>rd</sup> ed., 2017, part 2540 D  Standard Methods for the Examination of Water and Wastewater, APHA, AWWA & WEF, 23 <sup>rd</sup> ed., 2017, part 4500-F <sup>-</sup> C

ออกครั้งแรก ณ วันที่ 21 พฤศจิกายน 2560

ฉบับที่ 4

กองบริหารและรับรองห้องปฏิบัติการ กรมวิทยาศาสตร์บริการ กระทรวงการอุดมศึกษา วิทยาศาสตร์ วิจัย และนวัตกรรม

## ขอข่ายการรับรองความสามารถห้องปฏิบัติการทดสอบ

ชื่อห้องปฏิบัติการ : ห้องปฏิบัติการ บริษัท อีสเทิร์น ไทย คอนซัลต์ติ้ง 1992 จำกัด  
 สถานที่ตั้ง : เลขที่ 683 หมู่ที่ 11 ถนนสุขาภิบาล 8 ตำบลหนองขาม  
 อำเภอสรีราชา จังหวัดชลบุรี 20230

หมายเลขการรับรองระบบงานที่ : ทดสอบ - 0159

สถานะของห้องปฏิบัติการ : ☒ ถาวร ☐ นอกสถานที่ ☐ชั่วคราว ☐เคลื่อนที่

ลำดับ ที่	วัสดุ / ผลิตภัณฑ์ที่ทดสอบ	รายการที่ทดสอบ / ช่วงของการทดสอบ	วิธีทดสอบ / เทคนิคที่ใช้
2	น้ำเสีย	- ซีโอดี 40 mg/L ถึง 5 000 mg/L  - ปริมาณ 0.001 mg/L ถึง 0.02 mg/L  - บีโอดี 2 mg/L ถึง 5 000 mg/L	Standard Methods for the Examination of Water and Wastewater, APHA, AWWA & WEF, 23 <sup>rd</sup> ed., 2017, part 5220 C  Standard Methods for the Examination of Water and Wastewater, APHA, AWWA & WEF, 23 <sup>rd</sup> ed., 2017, part 3112 B  Standard Methods for the Examination of Water and Wastewater, APHA, AWWA & WEF, 23 <sup>rd</sup> ed., 2017, part 5210 B

ออกครั้งแรก ณ วันที่ 21 พฤศจิกายน 2560

ฉบับที่ 4

กองบริหารและรับรองห้องปฏิบัติการ กรมวิทยาศาสตร์บริการ กระทรวงการอุดมศึกษา วิทยาศาสตร์ วิจัย และนวัตกรรม

## ขอข่ายการรับรองความสามารถห้องปฏิบัติการทดสอบ

ชื่อห้องปฏิบัติการ : ห้องปฏิบัติการ บริษัท อีสเทิร์น ไทย คอนซัลตัง 1992 จำกัด

สถานที่ตั้ง : เลขที่ 683 หมู่ที่ 11 ถนนสุขาภิบาล 8 ตำบลหนองขาม

อำเภอศรีราชา จังหวัดชลบุรี 20230


หมายเลขการรับรองระบบงานที่ : ทดสอบ - 0159

สถานะของห้องปฏิบัติการ : ☒ ถาวร ☐ นอกสถานที่ ☐ชั่วคราว ☐เคลื่อนที่

ลำดับ ที่	วัสดุ / ผลิตภัณฑ์ที่ทดสอบ	รายการที่ทดสอบ / ช่วงของการทดสอบ	วิธีทดสอบ / เทคนิคที่ใช้
2 (ต่อ)	น้ำเสีย	- สารที่ละลายได้ทั้งหมด ที่อุณหภูมิ 180 °C 25 mg/L ถึง 10 000 mg/L  - สารแขวนลอยทั้งหมด ที่อุณหภูมิ 103 °C ถึง 105 °C 5 mg/L ถึง 2 000 mg/L  - ฟลูออไรด์ 0.5 mg/L ถึง 10 mg/L	Standard Methods for the Examination of Water and Wastewater, APHA, AWWA & WEF, 23 <sup>rd</sup> ed., 2017, part 2540 C  Standard Methods for the Examination of Water and Wastewater, APHA, AWWA & WEF, 23 <sup>rd</sup> ed., 2017, part 2540 D  Standard Methods for the Examination of Water and Wastewater, APHA, AWWA & WEF, 23 <sup>rd</sup> ed., 2017, part 4500-F <sup>-</sup> C

ออกให้ ณ วันที่ : 7 พฤศจิกายน 2566

ลงชื่อ :



(นางจันทร์น วรสรรพวิทย์)

นักวิทยาศาสตร์ชำนาญการพิเศษ

รักษาราชการแทน ผู้อำนวยการกองบริหารและรับรองห้องปฏิบัติการ

ออกครั้งแรก ณ วันที่ 21 พฤศจิกายน 2560

ฉบับที่ 4

กองบริหารและรับรองห้องปฏิบัติการ กรมวิทยาศาสตร์บริการ กระทรวงการอุดมศึกษา วิทยาศาสตร์ วิจัย และนวัตกรรม



แบบ กมช./สมอ.๒  
Form NSC/TISI 2

ใบรับรองเลขที่ 24-LB0026  
(Certificate No.)

## ใบรับรองระบบงาน

(Certificate of Accreditation)

อาศัยอำนาจตามความในพระราชบัญญัติการมาตรฐานแห่งชาติ พ.ศ. ๒๕๕๑  
(By Virtue of National Standardization Act B.E. 2551 (2008))

เลขาธิการสำนักงานมาตรฐานผลิตภัณฑ์อุตสาหกรรม  
(Secretary-General, Thai Industrial Standards Institute)

ออกใบรับรองฉบับนี้ให้  
(Issues this certificate to)

บริษัท ซีคอต จำกัด ฝ่ายห้องปฏิบัติการทดสอบด้านสิ่งแวดล้อม  
(Secot Company Limited, Environmental Laboratory Division)

ตั้งอยู่เลขที่  
(Address)

๒๓๙ ถนนริมคลองประปา แขวงบางซื่อ เขตบางซื่อ กรุงเทพมหานคร  
(239 Rimklongprapa Road, Bangsue, Bangkok)

ได้รับการรับรองความสามารถ  
(Certificate of competence)

ตามมาตรฐานเลขที่ มอก. ๑๗๐๒๕ - ๒๕๖๑  
(Standard No. TIS 17025-2561 (2018) (ISO/IEC 17025: 2017))

ข้อกำหนดทั่วไปว่าด้วยความสามารถของ ห้องปฏิบัติการทดสอบและห้องปฏิบัติการสอบเทียบ  
(General requirements for the competence of testing and calibration laboratories)

หมายเลขการรับรองที่ ทดสอบ ๐๓๙๔  
(Accreditation No. Testing 0394)

โดยมีรายละเอียดสาขาและขอบข่ายที่ใบรับรอง แสดงไว้ใน QR CODE และ [www.tisi.go.th](http://www.tisi.go.th)  
(Details of the scheme and scope of the certificate are shown in QR CODE and [www.tisi.go.th](http://www.tisi.go.th))

ออกให้ ณ วันที่ ๖ ธันวาคม พ.ศ. ๒๕๖๖  
(Issue date : 6 December B.E. 2566 (2023))

(นายวีระศักดิ์ เพ็งหล่ง)

ผู้อำนวยการสำนักงานคณะกรรมการการมาตรฐานแห่งชาติ  
ปฏิบัติราชการแทน

เลขาธิการสำนักงานมาตรฐานผลิตภัณฑ์อุตสาหกรรม



Signed by สำนักงานมาตรฐานผลิตภัณฑ์อุตสาหกรรม (สมอ.)  
Thai Industrial Standards Institute (TISI)  
Date: 2023-12-06T08:49:04.476+07:00

d68cb66b

กระทรวงอุตสาหกรรม สำนักงานมาตรฐานผลิตภัณฑ์อุตสาหกรรม  
(Ministry of Industry Thailand, Thai Industrial Standards Institute)



รายละเอียดสาขาและขอบข่ายใบรับรองห้องปฏิบัติการ  
(Scope of Accreditation for Testing)

ใบรับรองเลขที่ 24-LB0026  
(Certification No. 24-LB0026)



ชื่อห้องปฏิบัติการ  
(Laboratory Name)

บริษัท ซีคอต จำกัด ฝ่ายห้องปฏิบัติการทดสอบด้านสิ่งแวดล้อม  
(Secot Company Limited, Environmental Laboratory Division)

หมายเลขการรับรองที่  
(Accreditation No.)

ทดสอบ 0394  
(Testing 0394)

ฉบับที่ 02  
(Issue No.02)

ออกให้ตั้งแต่วันที่ 30 ตุลาคม พ.ศ. 2566  
(Valid from) (30 October B.E.2566 (2023))

ถึงวันที่ 8 กันยายน พ.ศ. 2571  
(Until) (8 September B.E.2571 (2028))

สถานภาพห้องปฏิบัติการ  
(Laboratory status)

☒ถาวร (Permanent) ☐นอกสถานที่ (Site) ☐ชั่วคราว (Temporary) ☐เคลื่อนที่ (Mobile) ☐หลายสถานที่ (Multisite)

สาขาการทดสอบ (Field of Testing)	รายการทดสอบ (Parameter)	วิธีทดสอบ (Test Method)
สาขาสังแวดล้อม (environmental field)  1. น้ำและน้ำเสีย (water and wastewater)	- โลหะหนัก (heavy metals)  • สารหนู (Arsenic, As) 0.000 5 mg/L ถึง 0.090 0 mg/L  • สารหนู (Arsenic, As) 0.05 mg/L ถึง 4.50 mg/L  • แบเรียม (Barium, Ba) 0.02 mg/L ถึง 4.50 mg/L  • แคดเมียม (Cadmium, Cd) 0.01 mg/L ถึง 4.50 mg/L  • โครเมียม (Chromium, Cr) 0.01 mg/L ถึง 4.50 mg/L	- Standard Methods for the Examination of Water and Wastewater, APHA, AWWA, WEF, 23 <sup>rd</sup> edition, 2017, Part 3030 F and Part 3114 C  - Standard Methods for the Examination of Water and Wastewater, APHA, AWWA, WEF, 23 <sup>rd</sup> edition, 2017, Part 3030 E and Part 3120 B

กระทรวงอุตสาหกรรม สำนักงานมาตรฐานผลิตภัณฑ์อุตสาหกรรม  
(Ministry of Industry, Thai Industrial Standards Institute)

หน้าที่ 1/9

รายละเอียดสาขาและขอบข่ายใบรับรองห้องปฏิบัติการ

(Scope of Accreditation for Testing)

ใบรับรองเลขที่ 24-LB0026

(Certification No. 24-LB0026)



ฉบับที่ 02  
(Issue No.02)

ออกให้ตั้งแต่วันที่ 30 ตุลาคม พ.ศ. 2566  
(Valid from) (30 October B.E.2566 (2023))

ถึงวันที่ 8 กันยายน พ.ศ. 2571  
(Until) (8 September B.E.2571 (2028))

สถานภาพห้องปฏิบัติการ  
(Laboratory status)

☒ ถาวร  
(Permanent)

☐ นอกสถานที่  
(Site)

☐ชั่วคราว  
(Temporary)

☐เคลื่อนที่  
(Mobile)

☐หลายสถานที่  
(Multisite)

สาขาการทดสอบ (Field of Testing)	รายการทดสอบ (Parameter)	วิธีทดสอบ (Test Method)
<p>สาขาส่งแวดล้อม (environmental field)</p> <p>1. น้ำและน้ำเสีย (ต่อ) (water and wastewater) (cont.)</p>	<p>- โลหะหนัก (heavy metals)</p> <ul style="list-style-type: none"> <li>ทองแดง (Copper, Cu) 0.02 mg/L ถึง 4.50 mg/L</li> <li>เหล็ก (Iron, Fe) 0.05 mg/L ถึง 9.00 mg/L</li> <li>ตะกั่ว (Lead, Pb) 0.03 mg/L ถึง 4.50 mg/L</li> <li>แมงกานีส (Manganese, Mn) 0.01 mg/L ถึง 9.00 mg/L</li> <li>นิกเกิล (Nickel, Ni) 0.01 mg/L ถึง 4.50 mg/L</li> <li>สังกะสี (Zinc, Zn) 0.02 mg/L ถึง 9.00 mg/L</li> </ul>	<p>- Standard Methods for the Examination of Water and Wastewater, APHA , AWWA, WEF, 23<sup>rd</sup> edition , 2017, Part 3030 E and Part 3120 B</p>

รายละเอียดสาขาและขอบข่ายใบรับรองห้องปฏิบัติการ

(Scope of Accreditation for Testing)

ใบรับรองเลขที่ 24-LB0026

(Certification No. 24-LB0026)



ฉบับที่ 02  
(Issue No.02)

ออกให้ตั้งแต่วันที่ 30 ตุลาคม พ.ศ. 2566  
(Valid from) (30 October B.E.2566 (2023))

ถึงวันที่ 8 กันยายน พ.ศ. 2571  
(Until) (8 September B.E.2571 (2028))

สถานภาพห้องปฏิบัติการ  
(Laboratory status)

☒ ถาวร  
(Permanent)

☐นอกสถานที่  
(Site)

☐ชั่วคราว  
(Temporary)

☐เคลื่อนที่  
(Mobile)

☐หลายสถานที่  
(Multisite)

สาขาการทดสอบ (Field of Testing)	รายการทดสอบ (Parameter)	วิธีทดสอบ (Test Method)
<p>สาขาส่งแวดล้อม (environmental field)</p> <p>1. น้ำและน้ำเสีย (ต่อ) (water and wastewater) (cont.)</p>	<p>- ซีโอดี (Chemical oxygen demand, COD) 100 mg/L ถึง 4 000 mg/L</p>	<p>- Standard Methods for the Examination of Water and Wastewater, APHA, AWWA, WEF, 23<sup>rd</sup> edition , 2017, Part 5220 D</p>
<p>2. บริเวณทำงาน (workplace)</p>	<p>- ฝุ่นละอองรวม (Total dust) 0.10 mg/filter ถึง 2.00 mg/filter</p> <p>- ฝุ่นละอองขนาดเล็ก (Respirable dust) 0.10 mg/filter ถึง 2.00 mg/filter</p>	<p>- NIOSH Manual of Analytical Methods (NMAM) , method 0500, 4<sup>th</sup> edition , 15<sup>th</sup> August 1994 (Exclude Sampling)</p> <p>- NIOSH Manual of Analytical Methods (NMAM) , method 0600, 4<sup>th</sup> edition , 15<sup>th</sup> January 1998 (Exclude Sampling)</p>



รายละเอียดสาขาและขอบข่ายใบรับรองห้องปฏิบัติการ  
(Scope of Accreditation for Testing)

ใบรับรองเลขที่ 24-LB0026  
(Certification No. 24-LB0026)



ฉบับที่ 02  
(Issue No.02)

ออกให้ตั้งแต่วันที่ 30 ตุลาคม พ.ศ. 2566  
(Valid from) (30 October B.E.2566 (2023))

ถึงวันที่ 8 กันยายน พ.ศ. 2571  
(Until) (8 September B.E.2571 (2028))

สถานภาพห้องปฏิบัติการ  
(Laboratory status)

☒ถาวร  
(Permanent)

☐นอกสถานที่  
(Site)

☐ชั่วคราว  
(Temporary)

☐เคลื่อนที่  
(Mobile)

☐หลายสถานที่  
(Multisite)

สาขาการทดสอบ (Field of Testing)	รายการทดสอบ (Parameter)	วิธีทดสอบ (Test Method)
<p>สาขาสังแวดล้อม (environmental field)</p> <p>2. บริเวณทำงาน (ต่อ) (workplace) (cont.)</p>	<ul style="list-style-type: none"> <li>เบนซีน (Benzene) 1.10 µg/tube ถึง 420 µg/tube</li> <li>โทลูอีน (Toluene) 1.10 µg/tube ถึง 420 µg/tube</li> <li>โทโครไซลีน (Total xylenes) 2.20 µg/tube ถึง 840 µg/tube</li> <li>เมตา, พารา-ไซลีน (m, p- Xylene) 1.10 µg/tube ถึง 420 µg/tube</li> <li>ออร์โธ-ไซลีน (o- Xylene) 1.10 µg/tube ถึง 420 µg/tube</li> </ul>	<ul style="list-style-type: none"> <li>NIOSH Manual of Analytical Methods (NMAM) , method 1501, 4<sup>th</sup> edition , 15<sup>th</sup> March 2003 (Exclude Sampling)</li> </ul>
<p>3. ปล่องระบายอากาศ (stack)</p>	<ul style="list-style-type: none"> <li>ซัลเฟอร์ไดออกไซด์ (Sulfur dioxide ) 1.00 mg/L ถึง 16 000 mg/L (solution)</li> </ul>	<ul style="list-style-type: none"> <li>US.EPA , Code of Federal Regulations , 40 CFR 60 appendix A , method 6 , July 2019 (Exclude Sampling)</li> </ul>

รายละเอียดสาขาและขอบข่ายใบรับรองห้องปฏิบัติการ  
(Scope of Accreditation for Testing)

ใบรับรองเลขที่ 24-LB0026  
(Certification No. 24-LB0026)



ฉบับที่ 02  
(Issue No.02)

ออกให้ตั้งแต่วันที่ 30 ตุลาคม พ.ศ. 2566  
(Valid from) (30 October B.E.2566 (2023))

ถึงวันที่ 8 กันยายน พ.ศ. 2571  
(Until) (8 September B.E.2571 (2028))

สถานภาพห้องปฏิบัติการ  
(Laboratory status)

☒ถาวร  
(Permanent)

☐นอกสถานที่  
(Site)

☐ชั่วคราว  
(Temporary)

☐เคลื่อนที่  
(Mobile)

☐หลายสถานที่  
(Multisite)

สาขาการทดสอบ (Field of Testing)	รายการทดสอบ (Parameter)	วิธีทดสอบ (Test Method)
<p>สาขาสังแวดล้อม (environmental field)</p> <p>3. ปล่องระบายอากาศ (ต่อ) (stack) (cont.)</p>	<ul style="list-style-type: none"> <li>ไฮโดรเจนฟลูออไรด์ (Hydrogen fluoride) 5 µg/sample ถึง 400 µg/sample</li> <li>ไฮโดรเจนคลอไรด์ (Hydrogen chloride) 5 µg/sample ถึง 400 µg/sample</li> </ul>	<ul style="list-style-type: none"> <li>WI-7.2-1-22 based on US.EPA , Code of Federal Regulations , 40 CFR 60 appendix A, method 26 , 2019 (Exclude Sampling)</li> </ul>

รายละเอียดสาขาและขอบข่ายใบรับรองห้องปฏิบัติการ  
(Scope of Accreditation for Testing)

ใบรับรองเลขที่ 24-LB0026  
(Certification No. 24-LB0026)



ฉบับที่ 02  
(Issue No.02)

ออกให้ตั้งแต่วันที่ 30 ตุลาคม พ.ศ. 2566  
(Valid from) (30 October B.E.2566 (2023))

ถึงวันที่ 8 กันยายน พ.ศ. 2571  
(Until) (8 September B.E.2571 (2028))

สถานภาพห้องปฏิบัติการ  
(Laboratory status)

☒ถาวร  
(Permanent)

☒นอกสถานที่  
(Site)

☐ชั่วคราว  
(Temporary)

☐เคลื่อนที่  
(Mobile)

☐หลายสถานที่  
(Multisite)

สาขาการทดสอบ (Field of Testing)	รายการทดสอบ (Parameter)	วิธีทดสอบ (Test Method)
<p>สาขาสังแวดล้อม (environmental field)</p> <p>4. บรรยากาศทั่วไป (ambient air)</p>	<p>- สารอินทรีย์ระเหยง่าย (Volatile organic compounds, VOCs)</p> <ul style="list-style-type: none"> <li>คลอโรอีthin (Chloroethene) 0.05 <math>\mu\text{g}/\text{m}^3</math> ถึง 51.00 <math>\mu\text{g}/\text{m}^3</math> (0.02 ppbv ถึง 20.00 ppbv)</li> <li>1,3-บิวทาไดเอิน (1,3-butadiene) 0.04 <math>\mu\text{g}/\text{m}^3</math> ถึง 44.00 <math>\mu\text{g}/\text{m}^3</math> (0.02 ppbv ถึง 20.00 ppbv)</li> <li>โบรมอมีเทน (Bromomethane) 0.08 <math>\mu\text{g}/\text{m}^3</math> ถึง 77.00 <math>\mu\text{g}/\text{m}^3</math> (0.02 ppbv ถึง 20.00 ppbv)</li> <li>อะครอลีน (Acrolein) 0.05 <math>\mu\text{g}/\text{m}^3</math> ถึง 45.00 <math>\mu\text{g}/\text{m}^3</math> (0.02 ppbv ถึง 20.00 ppbv)</li> </ul>	<p>- WI-7.2-1-24 based on US EPA , Compendium Method TO-15 , EPA/625/R-96/010b, Second edition, January 1999</p>

รายละเอียดสาขาและขอบข่ายใบรับรองห้องปฏิบัติการ  
(Scope of Accreditation for Testing)

ใบรับรองเลขที่ 24-LB0026  
(Certification No. 24-LB0026)



ฉบับที่ 02  
(Issue No.02)

ออกให้ตั้งแต่วันที่ 30 ตุลาคม พ.ศ. 2566  
(Valid from) (30 October B.E.2566 (2023))

ถึงวันที่ 8 กันยายน พ.ศ. 2571  
(Until) (8 September B.E.2571 (2028))

สถานภาพห้องปฏิบัติการ  
(Laboratory status)

☒ถาวร  
(Permanent)

☒นอกสถานที่  
(Site)

☐ชั่วคราว  
(Temporary)

☐เคลื่อนที่  
(Mobile)

☐หลายสถานที่  
(Multisite)

สาขาการทดสอบ (Field of Testing)	รายการทดสอบ (Parameter)	วิธีทดสอบ (Test Method)
<p>สาขาสังแวดล้อม (environmental field)</p> <p>4. บรรยากาศทั่วไป (ต่อ) (ambient air) (cont.)</p>	<p>- สารอินทรีย์ระเหยง่าย (Volatile organic compounds, VOCs)</p> <ul style="list-style-type: none"> <li>อะคริโลไนไตรล์ (Acrylonitrile) 0.04 <math>\mu\text{g}/\text{m}^3</math> ถึง 43.00 <math>\mu\text{g}/\text{m}^3</math> (0.02 ppbv ถึง 20.00 ppbv)</li> <li>ไดคลอโรมีเทน (Dichloromethane) 0.14 <math>\mu\text{g}/\text{m}^3</math> to 69.00 <math>\mu\text{g}/\text{m}^3</math> (0.04 ppbv ถึง 20.00 ppbv)</li> <li>คาร์บอนไดซัลไฟด์ (Carbon disulfide) 0.06 <math>\mu\text{g}/\text{m}^3</math> ถึง 62.00 <math>\mu\text{g}/\text{m}^3</math> (0.02 ppbv ถึง 20.00 ppbv)</li> <li>ไตรคลอโรมีเทน (Trichloromethane) 0.20 <math>\mu\text{g}/\text{m}^3</math> ถึง 97.00 <math>\mu\text{g}/\text{m}^3</math> (0.04 ppbv ถึง 20.00 ppbv)</li> <li>1,2-ไดคลอโรอีเทน (1,2-dichloroethane) 0.08 <math>\mu\text{g}/\text{m}^3</math> ถึง 80.00 <math>\mu\text{g}/\text{m}^3</math> (0.02 ppbv ถึง 20.00 ppbv)</li> </ul>	<p>- WI-7.2-1-24 based on US EPA , Compendium Method TO-15 , EPA/625/R-96/010b, Second edition, January 1999</p>

รายละเอียดสาขาและขอบข่ายใบรับรองห้องปฏิบัติการ  
(Scope of Accreditation for Testing)

ใบรับรองเลขที่ 24-LB0026  
(Certification No. 24-LB0026)



ฉบับที่ 02  
(Issue No.02)

ออกให้ตั้งแต่วันที่ 30 ตุลาคม พ.ศ. 2566  
(Valid from (30 October B.E.2566 (2023)))

ถึงวันที่ 8 กันยายน พ.ศ. 2571  
(Until) (8 September B.E.2571 (2028))

สถานภาพห้องปฏิบัติการ  
(Laboratory status)

☒ถาวร  
(Permanent)

☒นอกสถานที่  
(Site)

☐ชั่วคราว  
(Temporary)

☐เคลื่อนที่  
(Mobile)

☐หลายสถานที่  
(Multisite)

สาขาการทดสอบ (Field of Testing)	รายการทดสอบ (Parameter)	วิธีทดสอบ (Test Method)
<p>สาขาสีสิ่งแวดล้อม (environmental field)</p> <p>4. บรรยากาศทั่วไป (ต่อ) (ambient air) (cont.)</p>	<p>- สารอินทรีย์ระเหยง่าย (Volatile organic compounds ,VOCs)</p> <ul style="list-style-type: none"> <li>• เบนซีน (Benzene) 0.06 <math>\mu\text{g}/\text{m}^3</math> ถึง 63.00 <math>\mu\text{g}/\text{m}^3</math> (0.02 ppbv ถึง 20.00 ppbv)</li> <li>• คาร์บอนเตตระคลอไรด์ (Carbon tetrachloride) 0.25 <math>\mu\text{g}/\text{m}^3</math> ถึง 125 <math>\mu\text{g}/\text{m}^3</math> (0.04 ppbv ถึง 20.00 ppbv)</li> <li>• ไตรคลอโรเอทิลีน (Trichloroethylene) 0.21 <math>\mu\text{g}/\text{m}^3</math> ถึง 107 <math>\mu\text{g}/\text{m}^3</math> (0.04 ppbv ถึง 20.00 ppbv)</li> <li>• 1,2-ไดคลอโรโพรเพน (1,2-dichloropropane) 0.18 <math>\mu\text{g}/\text{m}^3</math> ถึง 92.00 <math>\mu\text{g}/\text{m}^3</math> (0.04 ppbv ถึง 20.00 ppbv)</li> <li>• เตตระคลอโรเอทิลีน (Tetrachloroethylene) 0.27 <math>\mu\text{g}/\text{m}^3</math> ถึง 135 <math>\mu\text{g}/\text{m}^3</math> (0.04 ppbv ถึง 20.00 ppbv)</li> </ul>	<p>- WI-7.2-1-24 based on US EPA , Compendium Method TO-15 , EPA/625/R-96/010b, Second edition, January 1999</p>

รายละเอียดสาขาและขอบข่ายใบรับรองห้องปฏิบัติการ  
(Scope of Accreditation for Testing)

ใบรับรองเลขที่ 24-LB0026  
(Certification No. 24-LB0026)



ฉบับที่ 02  
(Issue No.02)

ออกให้ตั้งแต่วันที่ 30 ตุลาคม พ.ศ. 2566  
(Valid from (30 October B.E.2566 (2023)))

ถึงวันที่ 8 กันยายน พ.ศ. 2571  
(Until) (8 September B.E.2571 (2028))

สถานภาพห้องปฏิบัติการ  
(Laboratory status)

☒ถาวร  
(Permanent)

☒นอกสถานที่  
(Site)

☐ชั่วคราว  
(Temporary)

☐เคลื่อนที่  
(Mobile)

☐หลายสถานที่  
(Multisite)

สาขาการทดสอบ (Field of Testing)	รายการทดสอบ (Parameter)	วิธีทดสอบ (Test Method)
<p>สาขาสีสิ่งแวดล้อม (environmental field)</p> <p>4. บรรยากาศทั่วไป (ต่อ) (ambient air) (cont.)</p>	<p>- สารอินทรีย์ระเหยง่าย (Volatile organic compounds ,VOCs)</p> <ul style="list-style-type: none"> <li>• 1,2-ไดโบรมโอเอเทน (1,2-dibromoethane) 0.31 <math>\mu\text{g}/\text{m}^3</math> ถึง 153 <math>\mu\text{g}/\text{m}^3</math> (0.04 ppbv ถึง 20.00 ppbv)</li> <li>• 1,1,2,2-เตตระคลอโรเอเทน (1,1,2,2-tetrachloroethane) 0.69 <math>\mu\text{g}/\text{m}^3</math> ถึง 137 <math>\mu\text{g}/\text{m}^3</math> (0.10 ppbv ถึง 20.00 ppbv)</li> <li>• เบนซิลคลอไรด์ (Benzyl chloride) 0.52 <math>\mu\text{g}/\text{m}^3</math> ถึง 103 <math>\mu\text{g}/\text{m}^3</math> (0.10 ppbv ถึง 20.00 ppbv)</li> <li>• 1,4-ไดคลอโรเบนซีน (1,4-dichlorobenzene) 0.24 <math>\mu\text{g}/\text{m}^3</math> ถึง 120 <math>\mu\text{g}/\text{m}^3</math> (0.04 ppbv ถึง 20.00 ppbv)</li> </ul>	<p>- WI-7.2-1-24 based on US EPA , Compendium Method TO-15 , EPA/625/R-96/010b, Second edition, January 1999</p>