

ภาคผนวก จ

เอกสารแสดงการตรวจเทียบเครื่องมือ
การติดตามตรวจสอบผลกระทบสิ่งแวดล้อม



High Volume TSP&PM10 Calibration Data Sheet

Date: 13 Jan 25

Temp (°C): 26

Barometric pressure (mm Hg): 761

Reference Standard Calibration

Equipment: Orifice

Model No: TE-5025A

Serial No: 4218

Manufacturer: Tisch

Unit Under Test


Equipment: High Volume Air Sampler

Model No: TE-5009X

Serial No: BH-017

Calibrated by : Surachat I.

Test No.	Orifice (in)	Qstd (m ³ /min)	Reading (in)	Reading(Corrected) (in)
1	12.78	1.710	7.86	7.85
2	10.71	1.567	6.39	6.38
3	8.11	1.366	4.95	4.94
4	5.25	1.104	3.32	3.32
5	3.29	0.878	2.02	2.02

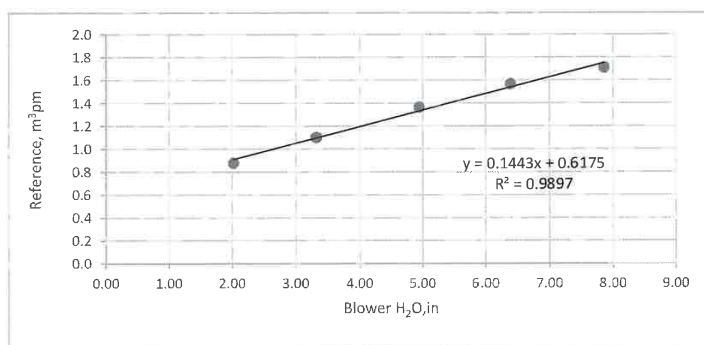

Approved by :



High Volume TSP&PM10 Calibration Data Sheet

Date: 10 Jan 25

Temp (°C): 30

Barometric pressure (mm Hg): 762

Reference Standard Calibration

Equipment: Orifice

Model No: TE-5025A

Serial No: 4218

Manufacturer: Tisch

Unit Under Test


Equipment: High Volume Air Sampler

Model No: TE-5009X

Serial No: BH-027

Calibrated by : Surachat I.

Test No.	Orifice (in)	Qstd (m ³ /min)	Reading (in)	Reading(Corrected) (in)
1	12.70	1.695	7.55	7.50
2	10.07	1.511	6.03	5.99
3	7.61	1.317	4.7	4.67
4	4.92	1.063	3.15	3.13
5	2.65	0.786	2.15	2.13

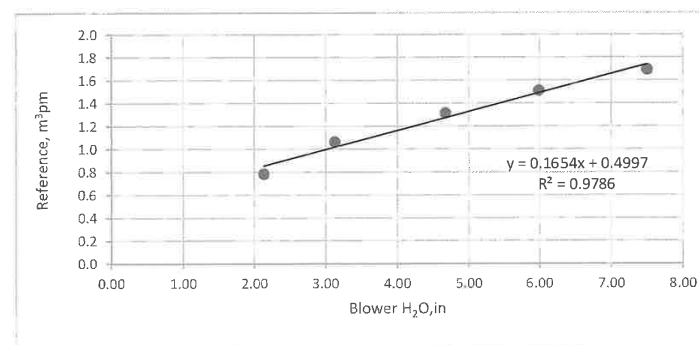

Approved by :

Sheet No. : BH-029-1/2025(P)



High Volume TSP&PM10 Calibration Data Sheet

Date: 13 Jan 25

Temp (°C): 26

Barometric pressure (mm Hg): 761

Reference Standard Calibration

Equipment: Orifice

Model No: TE-5025A

Serial No: 4218

Manufacturer: Tisch

Unit Under Test


Equipment: High Volume Air Sampler

Model No: TE-5009X

Serial No: BH-029

Calibrated by : Surachat I.

Test No.	Orifice (in)	Qstd (m ³ /min)	Reading (in)	Reading(Corrected) (in)
1	12.81	1.712	8.33	8.32
2	9.96	1.512	6.67	6.66
3	7.26	1.294	5.01	5.00
4	4.87	1.064	3.18	3.18
5	2.98	0.837	1.99	1.99

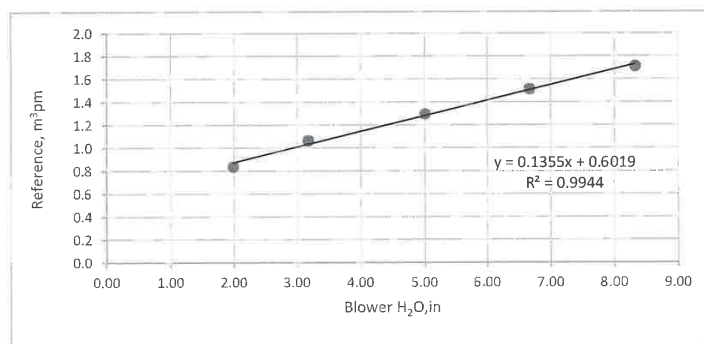

Approved by :

Airgas
an Air Liquide company

Airgas Specialty Gases
Airgas USA, LLC
600 Union Landing Road
Cinnaminson, NJ 08077-0000
Airgas.com

CERTIFICATE OF ANALYSIS

Grade of Product: EPA Protocol

Part Number: E04NI99E15AC084 Reference Number: 82-401409170-1
 Cylinder Number: EB0102326 Cylinder Volume: 144.4 CF
 Laboratory: 124 - Riverton (SAP) - NJ Cylinder Pressure: 2015 PSIG
 PGVP Number: B52019 Valve Outlet: 660
 Gas Code: CO,NO,NOX,SO₂,BALN Certification Date: Feb 05, 2019

Expiration Date: Feb 05, 2027

Certification performed in accordance with "EPA Traceability Protocol for Assay and Certification of Gaseous Calibration Standards (May 2012)" document EPA 600/R-12/531, using the assay procedures listed. Analytical Methodology does not require correction for analytical interference. This cylinder has a total analytical uncertainty as stated below with a confidence level of 95%. There are no significant impurities which affect the use of this calibration mixture. All concentrations are on a volume/volume basis unless otherwise noted.

Do Not Use This Cylinder below 100 psig, i.e. 0.7 megapascals.

ANALYTICAL RESULTS					
Component	Requested Concentration	Actual Concentration	Protocol Method	Total Relative Uncertainty	Assay Dates
NOX	50.00 PPM	51.01 PPM	G1	+/- 0.9% NIST Traceable	01/28/2019, 02/05/2019
NITRIC OXIDE	50.00 PPM	50.86 PPM	G1	+/- 0.9% NIST Traceable	01/28/2019, 02/05/2019
SULFUR DIOXIDE	50.00 PPM	50.87 PPM	G1	+/- 1.0% NIST Traceable	01/28/2019, 02/05/2019
CARBON MONOXIDE	0.5000 %	0.5050 %	G1	+/- 0.7% NIST Traceable	01/31/2019
NITROGEN	Balance				

CALIBRATION STANDARDS					
Type	Lot ID	Cylinder No	Concentration	Uncertainty	Expiration Date
NTRM	13060206	CC401947	4950 PPM CARBON MONOXIDE/NITROGEN	+/- 0.4%	Feb 15, 2019
PRM	12367	APEX1099237	9.82 PPM NITROGEN DIOXIDE/AIR	+/- 2.0%	Jun 02, 2017
NTRM	12010724	KAL004497	50.03 PPM NITRIC OXIDE/NITROGEN	+/- 0.8%	Mar 12, 2024
GMIS	1114201601	CC506710	4.971 PPM NITROGEN DIOXIDE/NITROGEN	+/- 2.0%	Nov 14, 2019
NTRM	14010327	KAL004378	49.08 PPM SULFUR DIOXIDE/NITROGEN	+/- 1.0%	Apr 17, 2024

The SRM, PRM or RGM noted above is only in reference to the GMIS used in the assay and not part of the analysis.

ANALYTICAL EQUIPMENT		
Instrument/Make/Model	Analytical Principle	Last Multipoint Calibration
Siemens Ultramat 6 J3-599 COHIGH	NDIR	Jan 18, 2019
Nicolet 6700 APW1100391 NO	FTIR	Jan 10, 2019
Nicolet 6700 APW1100391 NO2	FTIR	Jan 10, 2019
Nicolet 6700 APW1100391 SO2	FTIR	Jan 10, 2019

Triad Data Available Upon Request

PERMANENT NOTES: PRODUCED IN ACCORDANCE WITH ISO17025 REQUIREMENTS

NOTES:

Gross Weight: 27806.3 grams

Net Weight: 4733.2 grams

This calibration std. has been certified in accordance with the May 2012 EPA Traceability Protocol for Assay and Certification of Gaseous Calibration Standards (May 2012) document EPA-600/R-12/531. All testing processes and measurements conform to the requirements of ISO/IEC 17025 and to Airgas ISO 9001:2008 and relate only to items identified on this certificate. This certificate is not valid unless accompanied by the original certificate. This document shall not be reproduced in full without written approval of the issuer.


ACCREDITED

TESTING CERT No. 3082.05

Approved for Release

Page 1 of 82-401409170-1



CONTROL UNIT CALIBRATION

(Metric units, mm)

Date 6 Jan 25

Initial Final Average
Barometric press, Pb 758 758 758 mmHg

Dry Gas Meter Data

Console No. M50-06

Metering System ID

DGM Number 917415

DGM Model MST-C2-1

Calibrated by : Montri P.

Reference Dry Gas Meter Data

Serial No. 358794

Model S110

Correction factor (Yr) 1.0077

Last Calibration Date 25 Oct 24

Orifice manometer setting, ΔH mm H2O	Ref.	DGM	Temperature (°C)				Time ⊙ min	DGM Correction factor (Y)	ΔH@ mm
	DGM	Volume V _m Liters	Ref DGM T _r	Dry Gas Meter					
	Volume V _r Liters			Inlet T _i	Outlet T _o	Avg T _m			
12.5	100.0	99.8	25	25	24	24.5	8.92	1.0071	45.1453
25.0	100.2	100.4	25	25	24	24.5	6.13	1.0020	42.5581
50.0	100.0	100.9	25	25	24	24.5	4.33	0.9923	42.6407
76.0	100.1	102.5	25	25	24	24.5	3.53	0.9756	43.0400
100.0	100.1	102.2	25	25	24	24.5	3.53	0.9755	43.5926
150.0	100.0	101.5	25	25	24	24.5	2.53	0.9774	43.7294

Average 0.9883 43.4510

Approved by :



CONTROL UNIT CALIBRATION

(Metric units, mm)

Date 6 Jan 25

Initial Final Average
Barometric press, Pb 758 758 758 mmHg

Dry Gas Meter Data

Console No. M50-07

Metering System ID

DGM Number 90331

DGM Model MST-C2-1

Calibrated by Montri P.

Reference Dry Gas Meter Data

Serial No. 358794

Model S110

Correction factor (Yr) 1.0077

Last Calibration Date 25 Oct 24

Orifice manometer setting, ΔH mm H2O	Ref. DGM Volume V _r Liters	DGM Volume V _m Liters	Temperature (°C)				Time ⊙ min	DGM Correction factor (Y)	ΔH@ mm
			Ref DGM T _r	Dry Gas Meter					
				Inlet T _i	Outlet T _o	Avg T _m			
12.5	100.1	101.0	25	25	24	24.5	8.67	0.9958	42.5842
25.0	99.9	100.8	25	25	24	24.5	6.23	0.9946	44.2513
50.0	100.0	100.9	25	25	24	24.5	4.62	0.9920	48.4414
76.0	100.1	99.3	25	25	24	24.5	3.63	1.0074	45.4868
100.0	100.2	100.7	25	25	24	24.5	3.63	0.9921	47.7831
150.0	99.9	99.4	25	25	24	24.5	2.62	0.9970	46.7598

Average 0.9965 45.8844

Approved by :



PITOT TUBE CALIBRATION REPORT

Calibration Location: SECOT

Calibration Date : 04-01-2025

Calibration Duct No.: CD-0123

Calibration Standard Pitot tube data

Pitot No. : Std-02

Coefficient (Cp) : 0.99

Type S Pitot No. : LL10-01

Calibrated by : Mr. Montri P.

A Side Calibration

Run No.	ΔP_{std} (mm H ₂ O)	ΔP_s (mm H ₂ O)	Cp(s)	Deviation, δ Cp(s) - Cp(A)
1	15.0	21.0	0.8367	-0.0068
2	15.0	20.5	0.8468	0.0034
3	15.0	20.5	0.8468	0.0034

C_{P(A),avg} 0.8435

B Side Calibration

Run No.	ΔP_{std} (mm H ₂ O)	ΔP_s (mm H ₂ O)	Cp(s)	Deviation, δ Cp(s) - Cp(B)
1	15.0	20.5	0.8468	0.0034
2	15.0	21.0	0.8367	-0.0068
3	15.0	20.5	0.8468	0.0034

C_{P(B),avg} 0.8435

| CP(A)-CP(B) | = 0.0000

C_{P(Avg)} = 0.8435

Approved by :

*** δ must be ≤ 0.01 for the test to be acceptable ***
 *** | Cp(A)-Cp(B) | must also be < 0.01 if average of Cp(A) and Cp(B) is to be used ***



PITOT TUBE CALIBRATION REPORT

Calibration Location: SECOT

Calibration Date : 04-01-2025

Calibration Duct No.: CD-0123

Calibration Standard Pitot tube data

Pitot No. : Std-02

Coefficient (Cp) : 0.99

Type S Pitot No. : LL10-02

Calibrated by : Mr. Montri P.

A Side Calibration

Run No.	ΔP_{std} (mm H ₂ O)	ΔP_s (mm H ₂ O)	Cp(s)	Deviation, δ Cp(s) - Cp(A)
1	15.0	20.5	0.8468	-0.0035
2	15.0	20.5	0.8468	-0.0035
3	15.0	20.0	0.8574	0.0070

C_{P(A),avg} 0.8504

B Side Calibration

Run No.	ΔP_{std} (mm H ₂ O)	ΔP_s (mm H ₂ O)	Cp(s)	Deviation, δ Cp(s) - Cp(B)
1	15.0	20.5	0.8468	0.0034
2	15.0	21.0	0.8367	-0.0068
3	15.0	20.5	0.8468	0.0034

C_{P(B),avg} 0.8435

| CP(A)-CP(B) | = 0.0069

C_{P(Avg)} = 0.8469

Approved by :

*** δ must be ≤ 0.01 for the test to be acceptable ***
 *** | Cp(A)-Cp(B) | must also be < 0.01 if average of Cp(A) and Cp(B) is to be used ***



PITOT TUBE CALIBRATION REPORT

Calibration Location: SECOT

Calibration Date : 04-01-2025

Calibration Duct No.: CD-0123

Calibration Standard Pitot tube data

Pitot No. : Std-02

Coefficient (Cp) : 0.99

Type S Pitot No. : PD20-01

Calibrated by : Mr. Montri P.

A Side Calibration

Run No.	ΔP_{std} (mm H ₂ O)	ΔP_s (mm H ₂ O)	Cp(s)	Deviation, δ Cp(s) - Cp(A)
1	14.5	20.5	0.8326	-0.0034
2	14.5	20.5	0.8326	-0.0034
3	14.5	20.0	0.8430	0.0069

C_{P(A),avg} 0.8361

B Side Calibration

Run No.	ΔP_{std} (mm H ₂ O)	ΔP_s (mm H ₂ O)	Cp(s)	Deviation, δ Cp(s) - Cp(B)
1	14.5	20.5	0.8326	-0.0034
2	14.5	20.5	0.8326	-0.0034
3	14.5	20.0	0.8430	0.0069

C_{P(B),avg} 0.8361

| CP(A)-CP(B) | = 0.0000

C_{P(Avg)} = 0.8361

Approved by :

*** δ must be ≤ 0.01 for the test to be acceptable ***
 *** | Cp(A)-Cp(B) | must also be < 0.01 if average of Cp(A) and Cp(B) is to be used ***



PITOT TUBE CALIBRATION REPORT

Calibration Location: SECOT

Calibration Date : 03-01-2025

Calibration Duct No.: CD-0123

Calibration Standard Pitot tube data

Pitot No. : Std-02

Coefficient (Cp) : 0.99

Type S Pitot No. : PS10-01

Calibrated by : Mr. Montri P.

A Side Calibration

Run No.	ΔP_{std} (mm H ₂ O)	ΔP_s (mm H ₂ O)	Cp(s)	Deviation, δ Cp(s) - Cp(A)
1	15.0	21.0	0.8367	-0.0034
2	15.0	20.5	0.8468	0.0068
3	15.0	21.0	0.8367	-0.0034

C_{P(A),avg} 0.8401

B Side Calibration

Run No.	ΔP_{std} (mm H ₂ O)	ΔP_s (mm H ₂ O)	Cp(s)	Deviation, δ Cp(s) - Cp(B)
1	15.0	21.0	0.8367	-0.0034
2	15.0	20.5	0.8468	0.0068
3	15.0	21.0	0.8367	-0.0034

C_{P(B),avg} 0.8401

| CP(A)-CP(B) | = 0.0000

C_{P(Avg)} = 0.8401

Approved by :

*** δ must be ≤ 0.01 for the test to be acceptable ***
 *** | Cp(A)-Cp(B) | must also be < 0.01 if average of Cp(A) and Cp(B) is to be used ***



PITOT TUBE CALIBRATION REPORT

Calibration Location: SECOT

Calibration Date : 03-01-2025

Calibration Duct No.: CD-0123

Calibration Standard Pitot tube data

Pitot No. : Std-02

Coefficient (Cp) : 0.99

Type S Pitot No. : PS20-01

Calibrated by : Mr. Montri P.

A Side Calibration

Run No.	ΔP_{std} (mm H ₂ O)	ΔP_s (mm H ₂ O)	Cp(s)	Deviation, δ Cp(s) - Cp(A)
1	15.0	21.0	0.8367	-0.0034
2	15.0	20.5	0.8468	0.0068
3	15.0	21.0	0.8367	-0.0034

C_{P(A),avg} 0.8401

B Side Calibration

Run No.	ΔP_{std} (mm H ₂ O)	ΔP_s (mm H ₂ O)	Cp(s)	Deviation, δ Cp(s) - Cp(B)
1	15.0	21.0	0.8367	0.0065
2	15.0	21.5	0.8269	-0.0033
3	15.0	21.5	0.8269	-0.0033

C_{P(B),avg} 0.8302

| CP(A)-CP(B) | = 0.0099

C_{P(Avg)} = 0.8351Approved by : 

*** δ must be ≤ 0.01 for the test to be acceptable ***
 *** | Cp(A)-Cp(B) | must also be < 0.01 if average of Cp(A) and Cp(B) is to be used ***



PITOT TUBE CALIBRATION REPORT

Calibration Location: SECOT

Calibration Date : 03-01-2025

Calibration Duct No.: CD-0123

Calibration Standard Pitot tube data

Pitot No. : Std-02

Coefficient (Cp) : 0.99

Type S Pitot No. : PS20-02

Calibrated by : Mr. Montri P.

A Side Calibration

Run No.	ΔP_{std} (mm H ₂ O)	ΔP_s (mm H ₂ O)	Cp(s)	Deviation, δ Cp(s) - Cp(A)
1	15.0	20.5	0.8468	0.0000
2	15.0	20.5	0.8468	0.0000
3	15.0	20.5	0.8468	0.0000

C_{P(A),avg} 0.8468

B Side Calibration

Run No.	ΔP_{std} (mm H ₂ O)	ΔP_s (mm H ₂ O)	Cp(s)	Deviation, δ Cp(s) - Cp(B)
1	15.0	21.0	0.8367	-0.0034
2	15.0	21.0	0.8367	-0.0034
3	15.0	20.5	0.8468	0.0068

C_{P(B),avg} 0.8401

| CP(A)-CP(B) | = 0.0068

C_{P(Avg)} = 0.8435Approved by : 

*** δ must be ≤ 0.01 for the test to be acceptable ***
 *** | Cp(A)-Cp(B) | must also be < 0.01 if average of Cp(A) and Cp(B) is to be used ***

Certificate Of Analysis

Special Gases Mixture

Customer Details

Name: Secot Co., Ltd. Address: 239 Rimklongpropa Rd. Bangsue Khet Bangsue Bangkok 10800 Customer Tag No.:

Certificate Details

Number: 0483/23 Date of Issue: 22-Feb-2023 Expiry date: 21-Feb-2027
Material Details
Production Order: 90176403 Material Code: 478100-J-62 Cylinder No.: 51108
Gas content: 6.520 M³ (nominal) Filling pressure: 145 bar (g) Valve: CGA 590 BRASS
Cylinder Owner: LINDE Cylinder Material: STEEL Cylinder Size: 47 L

Laboratory Report

Component	Normal Concentration	Analysis Result ¹	Uncertainty ²	Method of Analysis ³
Oxygen	8.00%	7.93%	± 2% relative	(1) SG-O-01
In Nitrogen				

Recommend usage condition

Minimum utilization: 5% of actual content or before expiry date whichever comes first.
Storage condition: Keep in well ventilation and secure area.

Comments

Note:

- All results expressed in this report are on mole/mole basis, unless otherwise specified.
- The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor k=2, providing a level of confidence of approximately 95%. The measurement of this material is traceable to the SI through the reference gas standard which is traceable to Swiss National Standard of Mass or other recognised national metrology institutes.
- (1) Gas Chromatography, (2) Paramagnetic Oxygen Analyzer, (3) Electrochemical Oxygen Analyzer, (4) Electrochemical Moisture Analyzer, (5) Total Hydrocarbon Analyzer, (6) Other - Specified

Sukanya Parinyasontorn
Signatory for and on behalf of Linde (Thailand) Co., Ltd.

บริษัท ลินด์ (ประเทศไทย) จำกัด (มหาชน)

15 ชั้นตึกทาวเวอร์ เอ 2/3 หมู่ 14 ถนนบางนา-ตราด กม. 6.5 แขวงคลอง
บางพลี เขตสมุทรปราการ 10540 โทรศัพท์ (66) 2338-6100 โทรสาร (66) 2338-6333
โรงงานเวลโกรว์: 105 หมู่ 5 แขวงลำโพง อ.บางปะกง จ.ฉะเชิงเทรา 24180
โทรศัพท์ (66) 38.570-479-93 โทรสาร (66) 38.570-323

Linde (Thailand) Public Company Limited

P.C. Registration No. 0107537000785
15th Floor, Bangna Tower A, 2/3 Moo 14, Bangna Trd KM. 6.5 Road, Bangkaew
Bangplee, Samutprakarn 10540, Tel (66) 2338-6100 Fax (66) 2338-6333
Wellgrow Plant: 105 Moo 5, T.Bangamak, A.Bangpakong, Chachoengsao 24180
Thailand, Tel (66) 38.570-479-93 Fax (66) 38.570-323

Certificate Of Analysis

Special Gases Mixture

Customer Details

Name: Secot Co., Ltd. Address: 239 Rimklongpropa Rd. Bangsue Khet Bangsue Bangkok 10800 Customer Tag No.:

Certificate Details

Number: 0484/23 Date of Issue: 22-Feb-2023 Expiry date: 21-Feb-2027
Material Details
Production Order: 90176403 Material Code: 478100-J-62 Cylinder No.: 12360
Gas content: 6.520 M³ (nominal) Filling pressure: 145 bar (g) Valve: CGA 590 BRASS
Cylinder Owner: LINDE Cylinder Material: STEEL Cylinder Size: 47 L

Laboratory Report

Component	Normal Concentration	Analysis Result ¹	Uncertainty ²	Method of Analysis ³
Oxygen	8.00%	7.94%	± 2% relative	(1) SG-O-01
In Nitrogen				

Recommend usage condition

Minimum utilization: 5% of actual content or before expiry date whichever comes first.
Storage condition: Keep in well ventilation and secure area.

Comments

Note:

- All results expressed in this report are on mole/mole basis, unless otherwise specified.
- The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor k=2, providing a level of confidence of approximately 95%. The measurement of this material is traceable to the SI through the reference gas standard which is traceable to Swiss National Standard of Mass or other recognised national metrology institutes.
- (1) Gas Chromatography, (2) Paramagnetic Oxygen Analyzer, (3) Electrochemical Oxygen Analyzer, (4) Electrochemical Moisture Analyzer, (5) Total Hydrocarbon Analyzer, (6) Other - Specified

Sukanya Parinyasontorn
Signatory for and on behalf of Linde (Thailand) Co., Ltd.

บริษัท ลินด์ (ประเทศไทย) จำกัด (มหาชน)

15 ชั้นตึกทาวเวอร์ เอ 2/3 หมู่ 14 ถนนบางนา-ตราด กม. 6.5 แขวงคลอง
บางพลี เขตสมุทรปราการ 10540 โทรศัพท์ (66) 2338-6100 โทรสาร (66) 2338-6333
โรงงานเวลโกรว์: 105 หมู่ 5 แขวงลำโพง อ.บางปะกง จ.ฉะเชิงเทรา 24180
โทรศัพท์ (66) 38.570-479-93 โทรสาร (66) 38.570-323

Linde (Thailand) Public Company Limited

P.C. Registration No. 0107537000785
15th Floor, Bangna Tower A, 2/3 Moo 14, Bangna Trd KM. 6.5 Road, Bangkaew
Bangplee, Samutprakarn 10540, Tel (66) 2338-6100 Fax (66) 2338-6333
Wellgrow Plant: 105 Moo 5, T.Bangamak, A.Bangpakong, Chachoengsao 24180
Thailand, Tel (66) 38.570-479-93 Fax (66) 38.570-323

Making our world more productive



Certificate Of Analysis Special Gases Mixture

Customer Details

Name: Secot Co., Ltd. Address: 239, Rimklongprapa Rd., Bangsue, Bangkok 10800 Customer Tag No.:

Certificate Details

Number: 1393/24 Date of Issue: 24-May-2024 Expiry date: 24-May-2027
Material Details
Production Order: 90183672 Material Code: 436700-SK-34 Cylinder No.: A00987SK
Gas content: 6.900 M³ Filling pressure: 145 bar Valve: CGA 660 SS
Cylinder Owner: LINDE Cylinder Material: Spectra seal Cylinder Size: 40 L

Laboratory Report

Analytical Result

Component	Nominal Concentration	Analysis Result ¹	Uncertainty ²	Method of Analysis ³	Assay Date
Nitric Oxide	80.0 ppm	79.0 ppm	± 1% relative	(6) I-PB-352	15 & 23-May-2024
Other NOx impurity		Less Than 3.9 ppm			
Carbon Monoxide	80.0 ppm	81.7 ppm	± 1% relative	(6) I-PB-352	15 & 23-May-2024
In Nitrogen					

Reference Standard used in Assay

Reference Standard	Cylinder number	Concentration	Expiry date:
Carbon Monoxide	D619725	70.6 ± 0.2 ppm	20-Sep-2026
Nitric Oxide	D619725	70.6 ± 0.2 ppm	20-Sep-2026
In Nitrogen			

Analytical Instruments used in Assay

Instrument/Make/Model	Analytical Principle	Last Multipoint Calibration
FTIR Spectrometers Nicolet iS50	FTIR-CO	7-May-2024
FTIR Spectrometers Nicolet iS50	FTIR-NO	7-May-2024

Recommend usage condition

Minimum utilization: 5% of actual content or before expire date whichever comes first.

Storage condition: Keep in well ventilation and secure area.

Comments

When reordering, please quote the material number

Note:

- All results expressed in this report are on mole/mole basis, unless otherwise specified. The Assay of this Standard has been performed in accordance with the EPA Traceability Protocol EPA-600/R-12/531 for the Assay and Certification of Gaseous Calibration Standards using procedure G1.
- The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor k=2, providing a level of confidence of approximately 95%. The measurement of this material is traceable to the SI through the reference gas standard which is traceable to Swiss National Standard of Mass or other recognised national metrology institutes.
- (1) Gas Chromatography, (2) Paramagnetic Oxygen Analyzer, (3) Electrochemical Oxygen Analyzer, (4) Electrochemical Moisture Analyzer, (5) Total Hydrocarbon Analyzer, (6) Other - Specified

Page 1 of 1

This report shall not be reproduced except in full

Sukanya Parinyasoonorn

Signatory for and on behalf of Linde (Thailand) Co., Ltd.

PB-002/F006

Iss.M/1, 01 December 2023

บริษัท ลินด์ (ประเทศไทย) จำกัด (มหาชน)

เลขที่ใบอนุญาต: 0107537000783

ชั้น 15 อาคารทาวเวอร์ A, 2/3 หมู่ 14, ถนนบางนา-ตราด กม. 6.5, แขวงบางนา
แบริ่ง, เขตคลองเตย กรุงเทพมหานคร 10540 โทรศัพท์ (66) 2338-6100 โทรสาร (66) 2338-6333
โรงงานผลิต: 105 หมู่ 5 ตำบลบางนา อำเภอบางนา จังหวัดชลบุรี 24180
โทรศัพท์ (66) 38-570-479-93 โทรสาร (66) 38-570-323

Linde (Thailand) Public Company Limited

P.L.C. Registration No. 0107537000783

15th Floor, Bangna Tower A, 2/3 Moo 14, Bangna Trad KM. 6.5 Road, Bangkwaew
Bangplee, Samutprakarn 10540, Tel (66) 2338-6100 Fax (66) 2338-6333
Wellgrow Plant: 105 Moo 5, T.Bangsamak, A.Bangpakong, Chachoengsao 24180
Thailand, Tel (66) 38-570-479-93 Fax (66) 38-570-323

THE LINDE GROUP



Certificate Of Analysis Special Gases Mixture

Customer Details

Name: Secot Co., Ltd. Address: 239, Rimklongprapa Rd., Bangsue, Bangkok 10800 Customer Tag No.:

Certificate Details

Number: 0528/23 Date of Issue: 8-Mar-2023 Expiry date: 8-Mar-2026
Material Details
Production Order: 90176406 Material Code: S11600-SK-34 Cylinder No.: A00722SK
Gas content: 5.20 M³ Filling pressure: 137.0 bar Valve: CGA 660 SS
Cylinder Owner: LINDE Cylinder Material: Spectra seal Cylinder Size: 40 L

Laboratory Report

Analytical Result

Component	Nominal Concentration	Analysis Result ¹	Uncertainty ²	Method of Analysis ³	Assay Date
Nitric Oxide	40.0 ppm	39.6 ppm	± 1% relative	(6) I-PB-352	1-Mar & 8-Mar-2023
Other NOx impurity		Less than 1.9 ppm			
Carbon Monoxide	40.0 ppm	41.9 ppm	± 1% relative	(6) I-PB-352	1-Mar-2023
In Nitrogen					

Reference Standard used in Assay

Reference Standard	Cylinder number	Concentration	Expiry date:
Nitric Oxide	133261SG	25.61 ± 0.13 ppm	6-May-2023
Carbon Monoxide	ND52320	25.03 ± 0.13 ppm	7-Oct-2023
In Nitrogen			

Analytical Instruments used in Assay

Instrument/Make/Model	Analytical Principle	Last Multipoint Calibration
FTIR Spectrometers Nicolet iS50	FTIR-NO	28-Feb-2023
FTIR Spectrometers Nicolet iS50	FTIR-CO	25-Feb-2023

Recommend usage condition

Minimum utilization: 5% of actual content or before expire date whichever comes first.

Storage condition: Keep in well ventilation and secure area.

Comments

When reordering, please quote the material number

Note:

- All results expressed in this report are on mole/mole basis, unless otherwise specified. The Assay of this Standard has been performed in accordance with the EPA Traceability Protocol EPA-600/R-12/531 for the Assay and Certification of Gaseous Calibration Standards using procedure G1.
- The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor k=2, providing a level of confidence of approximately 95%. The measurement of this material is traceable to the SI through the reference gas standard which is traceable to Swiss National Standard of Mass or other recognised national metrology institutes.
- (1) Gas Chromatography, (2) Paramagnetic Oxygen Analyzer, (3) Electrochemical Oxygen Analyzer, (4) Electrochemical Moisture Analyzer, (5) Total Hydrocarbon Analyzer, (6) Other - Specified

Page 1 of 1

This report shall not be reproduced except in full

บริษัท ลินด์ (ประเทศไทย) จำกัด (มหาชน)

เลขที่ใบอนุญาต: 0107537000783

ชั้น 15 อาคารทาวเวอร์ A, 2/3 หมู่ 14, ถนนบางนา-ตราด กม. 6.5, แขวงบางนา
แบริ่ง, เขตคลองเตย กรุงเทพมหานคร 10540 โทรศัพท์ (66) 2338-6100 โทรสาร (66) 2338-6333
โรงงานผลิต: 105 หมู่ 5 ตำบลบางนา อำเภอบางนา จังหวัดชลบุรี 24180

Sukanya Parinyasoonorn

Signatory for and on behalf of Linde (Thailand) Co., Ltd.

PB-002/F006

Linde (Thailand) Public Company Limited Iss.K/2, 15 Oct 2021

P.L.C. Registration No. 0107537000783

15th Floor, Bangna Tower A, 2/3 Moo 14, Bangna Trad KM. 6.5 Road, Bangkwaew
Bangplee, Samutprakarn 10540, Tel (66) 2338-6100 Fax (66) 2338-6333
Wellgrow Plant: 105 Moo 5, T.Bangsamak, A.Bangpakong, Chachoengsao 24180

THE LINDE GROUP

Linde

Certificate Of Analysis
Special Gases Mixture

Customer Details

Name: Secot Co.,Ltd. Address: 239, Rimklongprapa Rd., Bangsue, Bangkok 10800 Customer Tag No.:

Certificate Details

Number: 0273/22 Date of Issue: 4-Feb-2022 Expiry date: 4-Feb-2030
Material Details
Production Order: 90169723 Material Code: 445100-SK-44 Cylinder No.: D636047
Gas content: 5.52 M³ Filling pressure: 145.0 bar Valve: CGA 660 SS
Cylinder Owner: LINDE Cylinder Material: Spectra seal Cylinder Size: 40 L

Laboratory Report

Analytical Result

Component	Normal Concentration	Analysis Result ¹	Uncertainty ²	Method of Analysis ³	Assay Date
Sulphur Dioxide In Nitrogen	80.0 ppm	81.0 ppm	± 1% relative	(6) I-PB-352	28-Jan & 4-Feb-22

Reference Standard used in Assay

Reference Standard	Cylinder number	Concentration	Expiry date:
Sulphur Dioxide In Nitrogen	256240	52.73 ± 0.42 ppm	6-May-2023

Analytical Instruments used in Assay

Instrument/Make/Model	Analytical Principle	Last Multipoint Calibration
FTIR Spectrometers Nicolet iS50	FTIR-SO2	10-Jan-2022

Recommend usage condition

Minimum utilization: 5% of actual content or before expiry date whichever comes first.
Storage condition: Keep in well ventilation and secure area.

Comments

When reordering, please quote the material number

Note:

1. All results expressed in this report are on mole/mole basis, unless otherwise specified. The Assay of this Standard has been performed in accordance with the EPA Traceability Protocol EPA-600/R-12/531 for the Assay and Certification of Gaseous Calibration Standards using procedure G1
2. The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor k=2, providing a level of confidence of approximately 95%. The measurement of this material is traceable to the SI through the reference gas standard which is traceable to Swiss National Standard of Mass or other recognised national metrology institutes.
3. (1) Gas Chromatography, (2) Paramagnetic Oxygen Analyzer, (3) Electrochemical Oxygen Analyzer, (4) Electrochemical Moisture Analyzer, (5) Total Hydrocarbon Analyzer, (6) Other - Specified

Sukanya Parinyasontorn
Signatory for and on behalf of Linde (Thailand) Co., Ltd.

Page 1 of 1

This report shall not be reproduced except in full

บริษัท ลินด์ (ประเทศไทย) จำกัด (มหาชน)

เลขที่ใบขึ้นทะเบียนมาตรฐาน 0107537000785

ชั้น 15 อาคารทาวเวอร์ เอ 2/3 หมู่ 14 ถนนบางนา-ตราด กม. 6.5 แขวงคลอง
บางพลี เขตสมุทรปราการ 10540 โทรศัพท์ (66) 2338-6100 โทรสาร (66) 2338-6333

โรงงานเวลโกรว์ : 105 หมู่ 5 ตำบลบางค้อ อำเภอบางพลี จังหวัดสมุทรปราการ 24180

โทรศัพท์ (66) 38.570-479-93

โทรสาร (66) 38.570-323

Linde (Thailand) Public Company Limited

PLC Registration no. 0107537000785

15th Floor, Bangna Tower A, 2/3 Moo 14, Bangna Trad KM. 6.5 Road, Bangkaew
Bangplee, Samutprakarn 10540, Tel (66) 2338-6100 Fax (66) 2338-6333

Wellgrow Plant: 105 Moo 5, T.Bangsamak, A.Bangpakong, Chachoengsao 24180

Thailand, Tel (66) 38.570-479-93

Fax (66) 38.570-323

PB-002/F006

Iss-K/2, 15 Oct 2021

THE LINDE GROUP

Linde

Certificate Of Analysis
Special Gases Mixture

Customer Details

Name: Secot Co.,Ltd. Address: 239, Rimklongprapa Rd., Bangsue, Bangkok 10800 Customer Tag No.:

Certificate Details

Number: 0275/22 Date of Issue: 4-Feb-2022 Expiry date: 4-Feb-2026
Material Details
Production Order: 90169722 Material Code: 631500-SK-44 Cylinder No.: D636195
Gas content: 5.52 M³ Filling pressure: 145.0 bar Valve: CGA 660 SS
Cylinder Owner: LINDE Cylinder Material: Spectra seal Cylinder Size: 40 L

Laboratory Report

Analytical Result

Component	Normal Concentration	Analysis Result ¹	Uncertainty ²	Method of Analysis ³	Assay Date
Sulphur Dioxide In Nitrogen	20.0 ppm	20.4 ppm	± 1% relative	(6) I-PB-352	28-Jan & 4-Feb-22

Reference Standard used in Assay

Reference Standard	Cylinder number	Concentration	Expiry date:
Sulphur Dioxide In Nitrogen	145754SG	25.03 ± 0.25 ppm	18-Aug-2022

Analytical Instruments used in Assay

Instrument/Make/Model	Analytical Principle	Last Multipoint Calibration
FTIR Spectrometers Nicolet iS50	FTIR-SO2	27-Jan-2022

Recommend usage condition

Minimum utilization: 5% of actual content or before expiry date whichever comes first.
Storage condition: Keep in well ventilation and secure area.

Comments

When reordering, please quote the material number

Note:

1. All results expressed in this report are on mole/mole basis, unless otherwise specified. The Assay of this Standard has been performed in accordance with the EPA Traceability Protocol EPA-600/R-12/531 for the Assay and Certification of Gaseous Calibration Standards using procedure G1
2. The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor k=2, providing a level of confidence of approximately 95%. The measurement of this material is traceable to the SI through the reference gas standard which is traceable to Swiss National Standard of Mass or other recognised national metrology institutes.
3. (1) Gas Chromatography, (2) Paramagnetic Oxygen Analyzer, (3) Electrochemical Oxygen Analyzer, (4) Electrochemical Moisture Analyzer, (5) Total Hydrocarbon Analyzer, (6) Other - Specified

Sukanya Parinyasontorn
Signatory for and on behalf of Linde (Thailand) Co., Ltd.

Page 1 of 1

This report shall not be reproduced except in full

บริษัท ลินด์ (ประเทศไทย) จำกัด (มหาชน)

เลขที่ใบขึ้นทะเบียนมาตรฐาน 0107537000785

ชั้น 15 อาคารทาวเวอร์ เอ 2/3 หมู่ 14 ถนนบางนา-ตราด กม. 6.5 แขวงคลอง
บางพลี เขตสมุทรปราการ 10540 โทรศัพท์ (66) 2338-6100 โทรสาร (66) 2338-6333

โรงงานเวลโกรว์ : 105 หมู่ 5 ตำบลบางค้อ อำเภอบางพลี จังหวัดสมุทรปราการ 24180

โทรศัพท์ (66) 38.570-479-93

โทรสาร (66) 38.570-323

PB-002/F006

Iss-K/2, 15 Oct 2021

Linde (Thailand) Public Company Limited

PLC Registration no. 0107537000785

15th Floor, Bangna Tower A, 2/3 Moo 14, Bangna Trad KM. 6.5 Road, Bangkaew
Bangplee, Samutprakarn 10540, Tel (66) 2338-6100 Fax (66) 2338-6333

Wellgrow Plant: 105 Moo 5, T.Bangsamak, A.Bangpakong, Chachoengsao 24180

Thailand, Tel (66) 38.570-479-93

Fax (66) 38.570-323

Sheet No. : CR-515-2025-116



SOUND LEVEL METER CALIBRATION

Calibration Location: SECOT

Calibration Date: Apr 28, 25

ACOUSTIC CALIBRATOR

Brand	Model	Serial No.	Frequency (Hz)	Ref.Calibrated (dB)	Eff.Calibrated (dB)
Cirrus	CR:515	97097	1000.00	94.0	93.7

No.	Brand	Model	Serial No.	Reading (dB)	dB Adjust
14	Cirrus	CR162B	G300709	93.7	0.0
20	Cirrus	CR162B	G301014	93.7	0.0
39	Cirrus	CR162B	G302743	93.7	0.0

Calibrated by :

Approved by :

Preeda S.

CR-515-2025-116/Cal/23/05/2025

SECOT CO., LTD.
239 Rimklongprapa Rd. Bangsue, Bangkok, 10800, THAILAND
Tel: (662) 959-3600 Fax: (662) 959-3535
E-Mail: envserv@secot.co.th



THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Mechanical Engineering Standards Laboratory Soi 1, Bangpoo Industrial Estate, Muang, Samutprakan 10280, Thailand.

Request No.23-68/0279

MTC.No.23-68/0279-01

Number of page(s) 2

CALIBRATION CERTIFICATE

Nomenclature : DRYCAL

Manufacturer : Mesa Labs

Serial No.: 160100

Model : Defender 520-L

Scale range : 5 ml/min to 500 ml/min

Subdivision : (0.001, 0.01) ml/min

Submitted by : SECOT CO.,LTD.

239, Rimklongprapa Road, Bangsue,

Bangkok 10800, Thailand.

Received date : 13 February 2025 Condition of measured item : Normal

Calibration date : 24 February 2025

Standard :

Standard	Certificate No.	Date due	Traceability
RTD Thermometer	PSL-T 0811/67	3-Jul-26	TISTR
Molbox/PressureTransducer/UpStream	MP-0076-23	2-Apr-25	NIMT
Primary Flow Calibrator S/N 117982	MW-0034-23	11-Jun-25	NIMT

Calibrated by : Terasak Panna

(Mr.Terasak Panna)

Approved by : Kirana Luanghirun

(Ms.Kirana Luanghirun)

Director

Mechanical Engineering Standards Laboratory

Ref. 2013268021300656001

Issued Date 28 February 2025

The results relate only to the items tested/calibrated or value assigned.
Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.5

Head Office

35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9009

Office/Laboratory

668 Mu 2 Tambon Bangpoomai, Amphoe Muang Samutprakan,
Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtc@tistr.or.th Website : www.tistr.or.th

Office

196 Phahonyothin Road, Ladyao, Chatuchak,
Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827



THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Mechanical Engineering Standards Laboratory Soi 1, Bangpoo Industrial Estate, Muang, Samutprakan 10280, Thailand.

Request No.23-68/0279

2/2

MTC.No.23-68/0279-01

Calibration point : (20, 50, 100, 200, 400) ml/min

Ambient condition : Temperature (23 ± 3) °C , Relative humidity (55 ± 15) %

Atmospheric pressure (1010 ± 13) hPa

Calibration method : The flowmeter (UUC) was calibrated by comparison method with standard flowmeter according to CP-370.01.

The reported value is the value that converted to value at reference condition within pressure and temperature of the actual gas entering the UUC

Measurement data :

UUC Value (ml/min)	Standard Value (ml/min)	Temperature (°C)	Pressure (hPa)	Deviation (%)	Uncertainty (%)
20.473*	20.340	24.275	1011.42	+0.65	0.94
49.952	50.732	24.057	1011.52	-1.54	0.95
99.449	99.622	24.102	1011.62	-0.17	0.93
200.34	199.94	24.133	1011.77	+0.20	0.93
401.89	397.98	24.140	1012.07	+0.98	0.93

The reported expanded uncertainties are based on standard uncertainties multiplied by a coverage factor $k=2$, which provides a level of confidence of approximately 95%.

* : The calibration point is not the scope of accreditation.

The end of calibration certificate.

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.5

Head Office

35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9009

Office/Laboratory

668 Mu 2 Tambon Bangpoo Mai, Amphoe Muang Samutprakan,
Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtc@tistr.or.th Website : www.tistr.or.th

Office

196 Phahonyothin Road, Ladyao, Chatuchak,
Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827



THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Mechanical Engineering Standards Laboratory Soi 1, Bangpoo Industrial Estate, Muang, Samutprakan 10280, Thailand.

Request No.23-68/0279

MTC.No.23-68/0279-02

Number of page(s) 2

CALIBRATION CERTIFICATE

Nomenclature : DRYCAL

Manufacturer : Mesa Labs

Serial No.: 114069

Model : Defender 520-H

Scale range : 300 ml/min to 30,000 ml/min

Subdivision : (0.0001, 0.001) L/min

Submitted by : SECOT CO.,LTD.

239, Rimklongprapa Road, Bangsue,

Bangkok 10800, Thailand.

Received date : 13 February 2025 **Condition of measured item :** Normal

Calibration date : 25 February 2025

Standard :

Standard	Certificate No.	Date due	Traceability
RTD Thermometer	PSL-T 0811/67	3-Jul-26	TISTR
Molbox/Pressure Transducer/UpStream	MP-0076-23	2-Apr-25	NIMT
Primary Flow Calibrator S/N 119216	MW-0035-23	31-May-25	NIMT

Calibrated by : Terasak Panna

(Mr.Terasak Panna)

Approved by : Ms. Kirana Luanghirun

(Ms.Kirana Luanghirun)

Director

Mechanical Engineering Standards Laboratory

Ref. 2013268021300656002

Issued Date 28 February 2025

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.5

Head Office

35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9009

Office/Laboratory

668 Mu 2 Tambon Bangpoo Mai, Amphoe Muang Samutprakan,
Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtc@tistr.or.th Website : www.tistr.or.th

Office

196 Phahonyothin Road, Ladyao, Chatuchak,
Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827



THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Mechanical Engineering Standards Laboratory Soi 1, Bangpoo Industrial Estate, Muang, Samutprakan 10280, Thailand.

Request No.23-68/0279

2/2

MTC.No.23-68/0279-02

Calibration point : (1.5, 5.0, 10, 15, 25) l/min

Ambient condition : Temperature (23 ± 3) °C , Relative humidity (55 ± 15) %

Atmospheric pressure (1010 ± 13) hPa

Calibration method : The flowmeter (UUC) was calibrated by comparison method with standard flowmeter according to CP-370.01.

The reported value is the value that converted to value at reference condition within pressure and temperature of the actual gas entering the UUC

Measurement data :

UUC Value	Standard Value	Temperature	Pressure	Deviation	Uncertainty
(L/min)	(L/min)	(°C)	(hPa)	(%)	(%)
1.5010	1.4862	24.354	1011.40	+0.99	0.91
5.0202	4.9882	24.364	1013.95	+0.64	0.89
9.9989	9.9228	24.319	1020.22	+0.77	0.89
15.033	14.819	24.342	1030.37	+1.44	0.89
25.136	24.152	24.331	1061.30	+4.08	0.89

The reported expanded uncertainties are based on standard uncertainties multiplied by a coverage factor $k=2$, which provides a level of confidence of approximately 95%.

The end of calibration certificate.

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

Head Office

35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9009

Office/Laboratory

668 Mu 2 Tambon Bangpoomai, Amphoe Muang Samutprakan,
Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtc@tistr.or.th Website : www.tistr.or.th

Office

196 Phahonyothin Road, Ladyao, Chatuchak,
Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827

FM.BL.MTC.002 Rev.5

Sheet No. : CAL-2505-0037-01



SOUND LEVEL METER CALIBRATION

Calibration Location: SECOT

Calibration Date: 26/05/2025

ACOUSTIC CALIBRATOR

Brand	Model	Serial No.	Frequency (Hz)	Ref.Calibrated (dB)	Eff.Calibrated (dB)
Cirrus	CR:515	94296	1000.00	94	93.8

No.	Brand	Model	Serial No.	Reading (dB)	dB Adjust
1	SCARLET TECH	ST-21D	820728	93.8	0.0
2	SCARLET TECH	ST-21D	820724	93.8	0.0
3	SCARLET TECH	ST-21D	820723	93.8	0.0
4	SCARLET TECH	ST-21D	820727	93.8	0.0
5	SCARLET TECH	ST-21D	820726	93.8	0.0
6	SCARLET TECH	ST-21D	820729	93.8	0.0

Calibrated by :

Approved by :

CER_PITGCS_2505-0037_Leq/Cal/21-06-25

SECOT CO., LTD.
239 Rinklongrogo Rd. Bangpue, Bangkok, 10600, THAILAND
Tel: (662)959-3600 Fax: (662) 959-3535
E-Mail: cnserv@secot.co.th

CERTIFICATE OF CALIBRATION

ISSUED BY Noisemeters

DATE OF ISSUE 26 February 2025 CERTIFICATE NUMBER 234084

NoiseMeters

NoiseMeters
Acoustic House
Bridlington Road
Hunmanby
YO14 0PH
United Kingdom
www.noisemeters.com

Page 1 of 2

Approved signatory
N.Smith
Electronically signed:



doseBadge Reader : IEC 60942:2003

Instrument information

Manufacturer: Cirrus Research plc

Notes:

Model: RC:110A

Serial number: 95167

Class: 2

Test summary

Date of calibration: 21 February 2025

The doseBadge reader detailed above has been calibrated to the published data as described in the operating manual and in the half-inch configuration. The procedures and techniques used are as described in IEC60942_2003 Annex B – Periodic Tests and three determinations of the sound pressure level, frequency and total distortion were made.

The sound pressure level was measured using a WS2F condenser microphone type MK:224 manufactured by Cirrus Research plc.

The results have been corrected to the reference pressure of 101.33 kPa using the manufacturer's data.

The doseBadge Reader has been shown to conform to the Class 2 requirements for periodic testing, described in Annex B of IEC 60942:2003 for the sound pressure level(s) and frequency(ies) stated, for the environmental conditions under which the tests were performed.

However, as public evidence was not available, from a testing organisation responsible for pattern approval, to demonstrate that the model of doseBadge Reader conformed to the requirements for pattern evaluation described in Annex A of IEC 60942:2003, no general statement or conclusion can be made about conformance of the doseBadge Reader to the requirements of IEC 60942:2003.

Notes:

This certificate provides traceability of measurement to the SI system of units and/or to units of measurement realised at the National Physical Laboratory or other recognised national metrology institutes. This certificate may not be reproduced other than in full, except with the prior written approval of the issuing laboratory. The results within this certificate relate only to the items calibrated. The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor k=2, providing a coverage probability of approximately 95%.

CERTIFICATE OF CALIBRATION

Certificate Number:

234084

Page 2 of 2

Environmental conditions

The following conditions were recorded at the time of the test:

Before Pressure: 99.38 kPa Temperature: 25.0 °C Humidity: 40.4 %
After Pressure: 99.39 kPa Temperature: 25.1 °C Humidity: 37.9 %

Test equipment

Equipment	Manufacturer	Model	Serial number
Distortion Meter	Keithley	2015	1063074
Environmental Monitor	Comet	T7510	21962628

Initial Acoustic Results

	Expected	Sample 1	Sample 2	Sample 3	Average	Deviation	Tolerance	Uncertainty
Level (dB)	114.00	113.79	113.78	113.79	113.79	-0.21	±0.75	0.11 dB
Distortion (%)	< 4.00	1.52	0.51	0.51	0.84	0.84	+4.00	0.13 %
Frequency (Hz)	1000.0	990.4	990.4	990.3	990.4	-9.6	±20.0	0.1 Hz

The measured quantities or deviations (as applicable), extended by the expanded combined uncertainty of measurement, must not exceed the corresponding tolerance.

Adjusted Acoustic Results

	Expected	Sample 1	Sample 2	Sample 3	Average	Deviation	Tolerance	Uncertainty
Level (dB)	114.00	113.97	113.97	113.97	113.97	-0.03	±0.75	0.11 dB
Distortion (%)	< 4.00	0.51	0.50	0.51	0.51	0.51	+4.00	0.13 %
Frequency (Hz)	1000.0	990.3	990.3	990.3	990.3	-9.7	±20.0	0.1 Hz

Functionality Results

Function	Result
Keypad	Pass
Battery Power	Pass
Display	Pass
Communication	Pass
2 way IR link	Pass
Clock	Pass

End of results

ภาคผนวก จ

ใบอนุญาตขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน
จากกรมโรงงานอุตสาหกรรม



ที่ อก ๐๓๑๐(๑)/ ๑๑ ๐๑ ๖

กรมโรงงานอุตสาหกรรม
ถนนพระรามที่ ๖ แขวงทุ่งพญาไท
เขตราชเทวี กรุงเทพฯ ๑๐๔๐๐

๒๐ กรกฎาคม ๒๕๖๖

เรื่อง ต่ออายุหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน

เรียน กรรมการผู้จัดการ บริษัท ซีคอต จำกัด

อ้างถึง คำขอขึ้นทะเบียน/ต่ออายุ/เปลี่ยนแปลงบุคลากร และชนิดสารมลพิษของห้องปฏิบัติการวิเคราะห์เอกชน
ลงวันที่ ๗ เมษายน ๒๕๖๖

- สิ่งที่ส่งมาด้วย ๑. รายชื่อผู้ควบคุมดูแลห้องปฏิบัติการวิเคราะห์ จำนวน ๑ แผ่น
๒. รายชื่อเจ้าหน้าที่ประจำห้องปฏิบัติการวิเคราะห์ จำนวน ๑ แผ่น
๓. ขอบข่ายสารมลพิษที่ได้รับขึ้นทะเบียนจากกรมโรงงานอุตสาหกรรม จำนวน ๓๙ แผ่น

ตามหนังสือที่อ้างถึง บริษัท ซีคอต จำกัด ขอต่ออายุหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน เลขทะเบียน ว-๒๓๙ สถานที่ตั้งเลขที่ ๒๓๙ ถนนริมคลองประปา แขวงบางซื่อ เขตบางซื่อ กรุงเทพมหานคร ต่อกรมโรงงานอุตสาหกรรม นั้น

กรมโรงงานอุตสาหกรรมพิจารณาแล้ว ให้บริษัท ซีคอต จำกัด ต่ออายุหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน โดยมีองค์ประกอบดังนี้

- ก. ผู้ควบคุมดูแลห้องปฏิบัติการวิเคราะห์ จำนวน ๑๐ ราย ตามสิ่งที่ส่งมาด้วย ๑
ข. เจ้าหน้าที่ประจำห้องปฏิบัติการวิเคราะห์ จำนวน ๓๘ ราย ตามสิ่งที่ส่งมาด้วย ๒
ค. ขอบข่ายสารมลพิษที่ได้รับขึ้นทะเบียนให้วิเคราะห์ในน้ำเสีย น้ำใต้ดิน อากาศเสีย สิ่งปฏิกูล หรือวัสดุที่ไม่ใช้แล้ว และดิน ตามสิ่งที่ส่งมาด้วย ๓

หนังสือฉบับนี้จะหมดอายุในวันที่ ๒ พฤษภาคม ๒๕๖๙ หากประสงค์จะต่ออายุหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน ให้ยื่นคำขอต่ออายุพร้อมเอกสารประกอบคำขอต่อกรมโรงงานอุตสาหกรรมภายใน ๓๐ วัน ก่อนวันสิ้นอายุของหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน ซึ่งคำขอต่ออายุดังกล่าวขอรับได้ที่กรมโรงงานอุตสาหกรรม ทั้งนี้ สามารถยื่นคำขอผ่านระบบอิเล็กทรอนิกส์ได้ที่หน้าเว็บไซต์กรมโรงงานอุตสาหกรรม

จึงเรียนมาเพื่อทราบ

ขอแสดงความนับถือ

(นายประสม ดำรงพงษ์)

กองวิจัยและเตือนภัยมลพิษโรงงาน
กลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษและทะเบียนห้องปฏิบัติการ
โทร. ๐ ๒๔๓๐ ๖๓๑๒ ต่อ ๒๑๐๓-๕
โทรสาร ๐ ๒๔๓๐ ๖๓๑๒ ต่อ ๒๑๔๙
ไปรษณีย์อิเล็กทรอนิกส์ saraban@diw.mail.go.th



“อุตสาหกรรมก้าวไกล ประเทศไทยก้าวหน้า ร่วมกันพัฒนา อุตสาหกรรมสีเขียว”



สิ่งที่ส่งมาด้วย ๑

เอกสารแนบท้ายหนังสือรับต่ออายุขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน

บริษัท ซีคอต จำกัด

เลขทะเบียน ว-๒๓๙

ที่ อก ๐๓๑๐(๑)/ ๑๑ ๐๑ ๖

ลงวันที่ ๒๐ กรกฎาคม ๒๕๖๖

ก. ผู้ควบคุมดูแลห้องปฏิบัติการวิเคราะห์ จำนวน ๑๐ ราย

- ๑) นายขรรชัย เกรียงไกรอุดม
๒) นางสมฤดี เกรียงไกรอุดม
๓) นางสาวธนา ทิพรักษ์
๔) นางสาวเมษุตา อินทร์ศรี
๕) นางสาวปรีดา สมใจ
๖) นางสาวอริญญา มาตา
๗) นางสาวลดาวัลย์ วงศ์เจริญ
๘) นางสาวณัฏฐวรรณ เกตวันดี
๙) นางสาวนริสา ภูวสรพีชญ์
๑๐) นางสาวศิริวรรณ ฉิมสง่า

- ทะเบียนเลขที่ ว-๒๓๙-ค-๐๐๐๒
ทะเบียนเลขที่ ว-๒๓๙-ค-๐๐๐๓
ทะเบียนเลขที่ ว-๒๓๙-ค-๐๐๐๔
ทะเบียนเลขที่ ว-๒๓๙-ค-๐๐๐๕
ทะเบียนเลขที่ ว-๒๓๙-ค-๐๐๐๖
ทะเบียนเลขที่ ว-๒๓๙-ค-๐๐๐๗
ทะเบียนเลขที่ ว-๒๓๙-ค-๐๐๐๘
ทะเบียนเลขที่ ว-๒๓๙-ค-๐๐๐๙
ทะเบียนเลขที่ ว-๒๓๙-ค-๐๐๑๐
ทะเบียนเลขที่ ว-๒๓๙-ค-๐๐๑๑

เอกสารแนบท้ายหนังสือรับต่ออายุขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน
บริษัท ชีคอฟ จำกัด

เลขทะเบียน ว-๒๓๙

ที่ อก ๐๓๑๐(๑)/ ๑๑๐๑ ๖

ลงวันที่ ๒๐ กรกฎาคม ๒๕๖๖

ข. เจ้าหน้าที่ประจำห้องปฏิบัติการวิเคราะห์ จำนวน ๓๘ ราย

๑) นางสาวสุดาพร สุนทร	ทะเบียนเลขที่	ว-๒๓๙-จ-๐๐๐๑
๒) นางสาวสุธาทิพย์ เทียนเตี้ย	ทะเบียนเลขที่	ว-๒๓๙-จ-๐๐๐๓
๓) นางสาวสุนันทา ศิริวัฒนานนท์	ทะเบียนเลขที่	ว-๒๓๙-จ-๐๐๐๔
๔) นายบวร ดีชัยยะ	ทะเบียนเลขที่	ว-๒๓๙-จ-๐๐๐๕
๕) นางสาวเกศรินทร์ วรเดโชวิทยา	ทะเบียนเลขที่	ว-๒๓๙-จ-๐๐๐๖
๖) นายอนันต์วัน พิมวันนา	ทะเบียนเลขที่	ว-๒๓๙-จ-๐๐๐๗
๗) นายชิตพล สมประสงค์	ทะเบียนเลขที่	ว-๒๓๙-จ-๐๐๐๘
๘) นางสาวศศิธร พรหมประเสริฐ	ทะเบียนเลขที่	ว-๒๓๙-จ-๐๐๐๙
๙) นายศิวนนท์ กุลวงษ์	ทะเบียนเลขที่	ว-๒๓๙-จ-๐๐๑๐
๑๐) นางสาวอลิษา คณิวรานนท์	ทะเบียนเลขที่	ว-๒๓๙-จ-๐๐๑๑
๑๑) นางสาวสิริวรรณ แก้วชิงดวง	ทะเบียนเลขที่	ว-๒๓๙-จ-๐๐๑๒
๑๒) นางสาวปัทมวรรณ สุวรรณวิโรจน์	ทะเบียนเลขที่	ว-๒๓๙-จ-๐๐๑๓
๑๓) นางสาวกนิษฐา เจริญเชื้อ	ทะเบียนเลขที่	ว-๒๓๙-จ-๐๐๑๔
๑๔) นายวัชรกานต์ ประมาคเต	ทะเบียนเลขที่	ว-๒๓๙-จ-๐๐๑๕
๑๕) นายชอง เฮงชวลกุล	ทะเบียนเลขที่	ว-๒๓๙-จ-๐๐๑๖
๑๖) นางสาวกฤษณา จันทุม	ทะเบียนเลขที่	ว-๒๓๙-จ-๐๐๑๗
๑๗) นางสาวพรนภา บุตรธรรม	ทะเบียนเลขที่	ว-๒๓๙-จ-๐๐๑๘
๑๘) นางสาวธาริณี อาจปลิว	ทะเบียนเลขที่	ว-๒๓๙-จ-๐๐๑๙
๑๙) นายอนันต์ ช่างลื้อ	ทะเบียนเลขที่	ว-๒๓๙-จ-๐๐๒๐
๒๐) นางสาวพัชรา สมานอันท์	ทะเบียนเลขที่	ว-๒๓๙-จ-๐๐๒๑
๒๑) นางสาวจุฑาทิพย์ แจ่มเรือน	ทะเบียนเลขที่	ว-๒๓๙-จ-๐๐๒๒
๒๒) นางสาวณิศา กุ้ยอ่อน	ทะเบียนเลขที่	ว-๒๓๙-จ-๐๐๒๓
๒๓) นายกิตติพงษ์ ณะเกิงสุข	ทะเบียนเลขที่	ว-๒๓๙-จ-๐๐๒๔
๒๔) นายจิรวัฒน์ โคตรคำหาญ	ทะเบียนเลขที่	ว-๒๓๙-จ-๐๐๒๕
๒๕) นายชนะพล อัครผล	ทะเบียนเลขที่	ว-๒๓๙-จ-๐๐๒๖
๒๖) นางสาวทิพย์สุดา วรรณการ	ทะเบียนเลขที่	ว-๒๓๙-จ-๐๐๒๗
๒๗) นายสิทธิชัย สว่างวงศ์ไชย	ทะเบียนเลขที่	ว-๒๓๙-จ-๐๐๒๘
๒๘) นายพิษณุ สีนามเพ็ง	ทะเบียนเลขที่	ว-๒๓๙-จ-๐๐๒๙
๒๙) นายรัตนชัย ขอบทำกิจ	ทะเบียนเลขที่	ว-๒๓๙-จ-๐๐๓๐
๓๐) นายธนาวุฒิ ด่วนแสง	ทะเบียนเลขที่	ว-๒๓๙-จ-๐๐๓๑
๓๑) นายณัฐชัย ไชยโคตร	ทะเบียนเลขที่	ว-๒๓๙-จ-๐๐๓๒
๓๒) นายณัฐดนัย กฤษณะโสม	ทะเบียนเลขที่	ว-๒๓๙-จ-๐๐๓๓
๓๓) นายศุภชัย สุขใหม่	ทะเบียนเลขที่	ว-๒๓๙-จ-๐๐๓๔
๓๔) นายรอมฎอน เหลี่ยมหมาด	ทะเบียนเลขที่	ว-๒๓๙-จ-๐๐๓๕
๓๕) นางสาวสุภาวดี บัวแก้ว	ทะเบียนเลขที่	ว-๒๓๙-จ-๐๐๓๖
๓๖) นางสาวมาริยาณี ฮาแว	ทะเบียนเลขที่	ว-๒๓๙-จ-๐๐๓๗
๓๗) นางสาววิระยา ปัจฉิมบุรณ์	ทะเบียนเลขที่	ว-๒๓๙-จ-๐๐๓๘
๓๘) นางสาวศลิษา อินริย์	ทะเบียนเลขที่	ว-๒๓๙-จ-๐๐๓๙

31/7/2566

เอกสารแนบท้ายหนังสือรับต่ออายุขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน
บริษัท ชีคอฟ จำกัด

เลขทะเบียน ว-๒๓๙

ที่ อก ๐๓๑๐(๑)/ ๑๑๐๑ ๖

ลงวันที่ ๒๐ กรกฎาคม ๒๕๖๖

ขอขยายสารมลพิษที่ได้รับขึ้นทะเบียนจากกรมโรงงานอุตสาหกรรม จำนวน ๓๕๕ รายการ

น้ำเสีย จำนวน 45 รายการ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
1	Aldrin	1) Liquid-Liquid Extraction, Gas Chromatographic Method ^[4] 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
2	Arsenic	1) Digestion, Hydride Generation/Atomic Absorption Spectrometric Method ^[4] 2) Digestion, Inductively Coupled Plasma Method ^[4]
3	Barium	1) Digestion, Direct Nitrous Oxide-Acetylene Flame Method ^[4] 2) Digestion, Inductively Coupled Plasma Method ^[4]
4	α-BHC	1) Liquid-Liquid Extraction, Gas Chromatographic Method ^[4] 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
5	β-BHC	1) Liquid-Liquid Extraction, Gas Chromatographic Method ^[4] 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
6	δ-BHC	1) Liquid-Liquid Extraction, Gas Chromatographic Method ^[4] 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
7	γ-BHC	1) Liquid-Liquid Extraction, Gas Chromatographic Method ^[4] 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]

31/7/2566

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
8	Biochemical Oxygen Demand	1) 5-Day BOD Test, Azide Modification Method ^[4] 2) 5-Day BOD Test, Membrane Electrode Method ^[4]
9	Cadmium	1) Digestion, Direct Air-Acetylene Flame Method ^[4] 2) Digestion, Electrothermal Atomic Absorption Spectrometric Method ^[4] 3) Digestion, Inductively Coupled Plasma Method ^[4]
10	Chemical Oxygen Demand	1) Open Reflux, Titrimetric method ^[4] 2) Closed Reflux, Colorimetric method ^[4] 3) Closed Reflux, Titrimetric Method ^[4]
11	Chlordane	1) Liquid-Liquid Extraction, Gas Chromatographic Method ^[4] 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
12	Chromium	1) Digestion, Direct Air-Acetylene Flame Method ^[4] 2) Digestion, Electrothermal Atomic Absorption Spectrometric Method ^[4] 3) Digestion, Inductively Coupled Plasma Method ^[4]
13	Color	ADMI Weighted-Ordinate Spectrophotometric Method ^[4]
14	Copper	1) Digestion, Direct Air-Acetylene Flame Method ^[4] 2) Digestion, Electrothermal Atomic Absorption Spectrometric Method ^[4] 3) Digestion, Inductively Coupled Plasma Method ^[4]
15	Cyanide	Distillation, Colorimetric method ^[4]
16	4,4'-DDD	1) Liquid-Liquid Extraction, Gas Chromatographic Method ^[4] 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]

17 4,4'-DDE...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
17	4,4'-DDE	1) Liquid-Liquid Extraction, Gas Chromatographic Method ^[4] 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
18	4,4'-DDT	1) Liquid-Liquid Extraction, Gas Chromatographic Method ^[4] 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
19	Dieldrin	1) Liquid-Liquid Extraction, Gas Chromatographic Method ^[4] 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
20	Endosulfan I	1) Liquid-Liquid Extraction, Gas Chromatographic Method ^[4] 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
21	Endosulfan II	1) Liquid-Liquid Extraction, Gas Chromatographic Method ^[4] 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
22	Endosulfan Sulfate	1) Liquid-Liquid Extraction, Gas Chromatographic Method ^[4] 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
23	Endrin	1) Liquid-Liquid Extraction, Gas Chromatographic Method ^[4] 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
24	Endrin Aldehyde	1) Liquid-Liquid Extraction, Gas Chromatographic Method ^[4] 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]

25 Formaldehyde...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
25	Formaldehyde	Distillation, Colorimetric Method ^[3]
26	Free Chlorine	1) Iodometric Method ^[4] 2) DPD Colorimetric Method ^[4]
27	Heptachlor	1) Liquid-Liquid Extraction, Gas Chromatographic Method ^[4] 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
28	Heptachlor epoxide	1) Liquid-Liquid Extraction, Gas Chromatographic Method ^[4] 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
29	Hexavalent Chromium	1) Colorimetric Method ^[4] 2) Extraction, Air-Acetylene Flame Method ^[4]
30	Lead	1) Digestion, Direct Air-Acetylene Flame Method ^[4] 2) Digestion, Electrothermal Atomic Absorption Spectrometric Method ^[4] 3) Digestion, Inductively Coupled Plasma Method ^[4]
31	Manganese	1) Digestion, Direct Air-Acetylene Flame Method ^[4] 2) Digestion, Electrothermal Atomic Absorption Spectrometric Method ^[4] 3) Digestion, Inductively Coupled Plasma Method ^[4]
32	Mercury	Digestion, Cold-Vapor Atomic Absorption Spectrometric Method ^[4]
33	Methoxychlor	1) Liquid-Liquid Extraction, Gas Chromatographic Method ^[4] 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
34	Nickel	1) Digestion, Direct Air-Acetylene Flame Method ^[4] 2) Digestion, Electrothermal Atomic Absorption Spectrometric Method ^[4]

3) Digestion...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
		3) Digestion, Inductively Coupled Plasma Method ^[4]
35	Oil & Grease	1) Liquid-Liquid, Partition-Gravimetric Method ^[4] 2) Soxhlet Extraction Method ^[4]
36	pH	Electrometric Method ^[4]
37	Phenols	1) Distillation, Chloroform Extraction Method ^[4] 2) Distillation, Direct Photometric Method ^[4]
38	Selenium	1) Digestion, Hydride Generation/Atomic Absorption Spectrometric Method ^[4] 2) Digestion, Inductively Coupled Plasma Method ^[4]
39	Sulfide	1) Iodometric method ^[4] 2) Methylene blue method ^[4]
40	Temperature	Laboratory and Field Methods ^[4]
41	Total Dissolved Solids	Dried at 180 °C ^[4]
42	Total Kjeldahl Nitrogen	1) Macro Kjeldahl Method ^[4] 2) Semi-Micro Kjeldahl Method ^[4]
43	Total Suspended Solids	Dried at 103-105 °C ^[4]
44	Trivalent Chromium	1) Digestion, Direct Air-Acetylene Flame Method; Colorimetric Method; Calculation ^[4] 2) Digestion, Electrothermal Atomic Absorption Spectrometric Method; Colorimetric Method; Calculation ^[4] 3) Digestion, Inductively Coupled Plasma Method; Colorimetric Method; Calculation ^[4]
45	Zinc	1) Digestion, Direct Air-Acetylene Flame Method ^[4] 2) Digestion, Electrothermal Atomic Absorption Spectrometric Method ^[4] 3) Digestion, Inductively Coupled Plasma Method ^[4]

น้ำใต้ดิน...

น้ำใต้ดิน จำนวน 125 รายการ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
1	Acenaphthene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
2	Acetone	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ^[4]
3	Aldrin	1) Liquid-Liquid Extraction, Gas Chromatographic Method ^[4] 2) Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
4	Anthracene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
5	Antimony	Digestion, Inductively Coupled Plasma Spectrometric Method ^[4]
6	Arsenic	1) Digestion, Hydride Generation/Atomic Absorption Spectrometric Method ^[4] 2) Digestion, Inductively Coupled Plasma Method ^[4]
7	Atrazine	Liquid-Liquid Extraction, Gas Chromatographic Method ^[4]
8	Barium	1) Digestion, Direct Nitrous Oxide-Acetylene Flame Method ^[4] 2) Digestion, Inductively Coupled Plasma Spectrometric Method ^[4]
9	Benz(a)anthracene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
10	Benzene	Purge and Trap Gas Chromatographic/Mass spectrometric Method ^[4]
11	Benzo(b)fluoranthene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
12	Benzo(k)fluoranthene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4] รั่ว)

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
13	Benzoic acid	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
14	Benzo(a)pyrene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
15	Benzo(g,h,i)perylene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
16	Beryllium	Digestion, Inductively Coupled Plasma Spectrometric Method ^[4]
17	Bis(2-chloroethyl)ether	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
18	Bis(2-ethylhexyl)phthalate	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
19	Bromodichloromethane	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ^[4]
20	Bromoform	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ^[4]
21	Butanol	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ^[4]
22	Butyl benzyl phthalate	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
23	Cadmium	1) Digestion, Direct Air-Acetylene Flame Method ^[4] 2) Digestion, Electrothermal Atomic Absorption Spectrometric Method ^[4] 3) Digestion, Inductively Coupled Plasma Spectrometric Method ^[4]
24	Carbazole	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
25	Carbon disulfide	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ^[4]
26	Carbon tetrachloride	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ^[4] รั่ว)

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
27	Chlordane	1) Liquid-Liquid Extraction, Gas Chromatographic Method ^[4] 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
28	p-Chloroaniline	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
29	Chlorobenzene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ^[4]
30	Chlorodibromomethane	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ^[4]
31	Chloroform	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ^[4]
32	2-Chlorophenol	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
33	Chromium	1) Digestion, Direct Air-Acetylene Flame Method ^[4] 2) Digestion, Electrothermal Atomic Absorption Spectrometric Method ^[4] 3) Digestion, Inductively Coupled Plasma Spectrometric Method ^[4]
34	Chromium (III)	1) Digestion, Direct Air-Acetylene Flame Method; Colorimetric Method; Calculation ^[4] 2) Digestion, Electrothermal Atomic Absorption Spectrometric Method; Colorimetric Method; Calculation ^[4] 3) Digestion, Inductively Coupled Plasma Spectrometric Method; Colorimetric Method; Calculation ^[4]
35	Chromium (VI)	1) Colorimetric Method ^[4] 2) Extraction, Air-Acetylene Flame Method ^[4]
36	Chrysene	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4] <i>simul</i>

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
37	Cyanide	1) Distillation, Titrimetric Method ^[4] 2) Distillation, Colorimetric Method ^[4]
38	2,4-D	Liquid-Liquid Extraction, Gas Chromatographic Method ^[4]
39	DDD	1) Liquid-Liquid Extraction, Gas Chromatographic Method ^[4] 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
40	DDE	1) Liquid-Liquid Extraction, Gas Chromatographic Method ^[4] 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
41	DDT	1) Liquid-Liquid Extraction, Gas Chromatographic Method ^[4] 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
42	Dibenz(a,h)anthracene	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
43	Di-n-butyl phthalate	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
44	1,2-Dichlorobenzene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ^[4]
45	1,3-Dichlorobenzene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ^[4]
46	1,4-Dichlorobenzene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ^[4]
47	3,3'-Dichlorobenzidine	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
48	1,1-Dichloroethane	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ^[4]
49	1,2-Dichloroethane	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ^[4] <i>simul</i>

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
50	1,1-Dichloroethylene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ^[4]
51	cis-1,2-Dichloroethylene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ^[4]
52	trans-1,2-Dichloroethylene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ^[4]
53	2,4-Dichlorophenol	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
54	1,2-Dichloropropane	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ^[4]
55	1,3-Dichloropropane	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ^[4]
56	1,3-Dichloropropene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ^[4]
57	Dieldrin	1) Liquid-Liquid Extraction, Gas Chromatographic Method ^[4] 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
58	Diethyl phthalate	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
59	2,4-Dimethylphenol	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
60	2,4-Dinitrophenol	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
61	2,4-Dinitrotoluene	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
62	2,6-Dinitrotoluene	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
63	Di-n-Octyl phthalate	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
64	Endosulfan	1) Liquid-Liquid Extraction, Gas Chromatographic Method ^[4] 2) Liquid-Liquid...

2) Liquid-Liquid...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
		2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
65	Endrin	1) Liquid-Liquid Extraction, Gas Chromatographic Method ^[4] 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
66	Ethylbenzene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ^[4]
67	Fluoranthene	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
68	Fluorene	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
69	Heptachlor	1) Liquid-Liquid Extraction, Gas Chromatographic Method ^[4] 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
70	Heptachlor epoxide	1) Liquid-Liquid Extraction, Gas Chromatographic Method ^[4] 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
71	Hexachlorobenzene	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
72	Hexachloro-1,3-butadiene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ^[4]
73	n-Hexane	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ^[4]
74	α-HCH	1) Liquid-Liquid Extraction, Gas Chromatographic Method ^[4] 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
75	β-HCH	1) Liquid-Liquid Extraction, Gas Chromatographic Method ^[4] 2) Liquid-Liquid...

2) Liquid-Liquid...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
76	γ-HCH	2) Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4] 1) Liquid-Liquid Extraction, Gas Chromatographic Method ^[4] 2) Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
77	Hexachlorocyclopentadiene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
78	Hexachloroethane	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
79	Indeno(1,2,3-cd)pyrene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
80	Isophorone	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
81	Lead	1) Digestion, Direct Air-Acetylene Flame Method ^[4] 2) Digestion, Electrothermal Atomic Absorption Spectrometric Method ^[4] 3) Digestion, Inductively Coupled Plasma Spectrometric Method ^[4]
82	Manganese	1) Digestion, Direct Air-Acetylene Flame Method ^[4] 2) Digestion, Electrothermal Atomic Absorption Spectrometric Method ^[4] 3) Digestion, Inductively Coupled Plasma Spectrometric Method ^[4]
83	Mercury	Digestion, Cold-Vapor Atomic Absorption Spectrometric Method ^[4]
84	Methanol	Purge and Trap Gas Chromatographic/ Mass spectrometric Method ^[4]
85	Methoxychlor	Liquid-Liquid Extraction, Gas Chromatographic Method ^[4]
86	Methyl bromide	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ^[4]

87 Methylene chloride...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
87	Methylene chloride	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ^[4]
88	2-Methylphenol	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
89	2-Methylnaphthalene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
90	Methyl tert-butyl ether	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ^[4]
91	Naphthalene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
92	Nickel	1) Digestion, Direct Air-Acetylene Flame Method ^[4] 2) Digestion, Electrothermal Atomic Absorption Spectrometric Method ^[4] 3) Digestion, Inductively Coupled Plasma Spectrometric Method ^[4]
93	Nitrobenzene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
94	N-Nitrosodiphenylamine	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
95	N-Nitrosodi-n-propylamine	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
96	Polychlorinated Biphenyls - PCB-1016 - PCB-1221 - PCB-1232 - PCB-1242 - PCB-1248 - PCB-1254 - PCB-1260	Liquid-Liquid Extraction, Gas Chromatographic Method ^[4]
97	Pentachlorophenol	Liquid-Liquid Extraction, Gas Chromatographic Method ^[4]
98	pH	Electrometric method ^[4]

99 Phenanthrene...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
99	Phenanthrene	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
100	Phenol	1) Distillation, Chloroform Extraction Method ^[4] 2) Distillation, Direct Photometric Method ^[4] 3) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
101	Pyrene	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
102	Selenium	1) Digestion, Hydride Generation/Atomic Absorption Spectrometric Method ^[4] 2) Digestion, Inductively Coupled Plasma Method ^[4]
103	Silver	1) Digestion, Direct Air-Acetylene Flame Method ^[4] 2) Digestion, Inductively Coupled Plasma Method ^[4]
104	Styrene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ^[4]
105	1,1,2,2-Tetrachloroethane	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ^[4]
106	Tetrachloroethylene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ^[4]
107	Toluene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ^[4]
108	TPH (C ₅ -C ₈)	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[12,25]
109	TPH (C ₈ -C ₁₆)	1) Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method ^[9,21] 2) Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass spectrometric Method ^[9,25]
110	TPH (C ₁₆ -C ₃₅)	1) Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method ^[9,21] <i>เพิ่ม</i>

2) Separatory...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
		2) Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass spectrometric Method ^[9,25]
111	1,2,4-Trichlorobenzene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ^[4]
112	1,1,1-Trichloroethane	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ^[4]
113	1,1,2-Trichloroethane	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ^[4]
114	Trichloroethylene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ^[4]
115	2,4,5-Trichlorophenol	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
116	2,4,6-Trichlorophenol	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
117	1,3,5-Trimethylbenzene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ^[4]
118	Vanadium	Digestion, Inductively Coupled Plasma Spectrometric Method ^[4]
119	Vinyl acetate	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ^[4]
120	Vinyl chloride	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ^[4]
121	m-Xylene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ^[4]
122	o-Xylene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ^[4]
123	p-Xylene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ^[4]
124	Xylene (Total)	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ^[4] <i>เพิ่ม</i>

125 Zinc ...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
125	Zinc	1) Digestion, Direct Air-Acetylene Flame Method ^[4] 2) Digestion, Electrothermal Atomic Absorption Spectrometric Method ^[4] 3) Digestion, Inductively Coupled Plasma Spectrometric Method ^[4]

อากาศเสีย (ปล่องระบาย) จำนวน 27 รายการ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
1	Antimony	1) Isokinetic Sampling, Digestion, Direct Air-Acetylene Flame Method ^[5] 2) Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method ^[5]
2	Arsenic	1) Isokinetic Sampling, Digestion, Hydride Generation/Atomic Absorption Spectrometric Method ^[5] 2) Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method ^[5]
3	Beryllium	Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method ^[5]
4	Cadmium	1) Isokinetic Sampling, Digestion, Direct Air-Acetylene Flame Method ^[5] 2) Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method ^[5]
5	Carbon monoxide	Instrumental Analyzer Method ^[5]
6	Chlorine	1) Absorption Sampling, Ion Chromatographic Method ^[5] 2) Isokinetic Sampling, Ion Chromatographic Method ^[5]
7	Chromium	1) Isokinetic Sampling, Digestion, Direct Air-Acetylene Flame Method ^[5] 2) Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method ^[5] <i>วิธีใหม่</i>

8 Cobalt...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
8	Cobalt	Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method ^[5]
9	Copper	1) Isokinetic Sampling, Digestion, Direct Air-Acetylene Flame Method ^[5] 2) Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method ^[5]
10	Cresol	Adsorption Sampling, Gas Chromatographic Method ^[5]
11	Dioxin/Furans	Isokinetic Sampling ^[5]
12	Hydrogen chloride	1) Absorption Sampling, Ion Chromatographic Method ^[5] 2) Isokinetic Sampling, Ion Chromatographic Method ^[5]
13	Hydrogen Fluoride	1) Absorption Sampling, Ion Chromatographic Method ^[5] 2) Isokinetic Sampling, Ion Chromatographic Method ^[5]
14	Hydrogen Sulfide	Absorption Sampling, Iodometric Method ^[5]
15	Lead	1) Isokinetic Sampling, Digestion, Direct Air-Acetylene Flame Method ^[5] 2) Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method ^[5]
16	Manganese	1) Isokinetic Sampling, Digestion, Direct Air-Acetylene Flame Method ^[5] 2) Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method ^[5]
17	Mercury	Isokinetic Sampling, Digestion, Cold-Vapor Atomic Absorption Spectrometric Method ^[5]
18	Nickel	1) Isokinetic Sampling, Digestion, Direct Air-Acetylene Flame Method ^[5] 2) Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method ^[5] <i>วิธีใหม่</i>

19 Opacity...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
19	Opacity	Ringelmann's Method ^[2]
20	Oxides of Nitrogen	1) Absorption Sampling, Phenoldisulfonic acid Method ^[5] 2) Absorption Sampling, Ion Chromatographic Method ^[5] 3) Instrumental Analyzer Method ^[5]
21	Selenium	1) Isokinetic Sampling, Digestion, Hydride Generation/Atomic Absorption Spectrometric Method ^[5] 2) Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method ^[5]
22	Sulfur dioxide	1) Isokinetic Sampling, Barium-Thorin Titrimetric Method ^[5] 2) Absorption Sampling, Barium-Thorin Titrimetric Method ^[5] 3) Instrumental Analyzer Method ^[5]
23	Sulfuric acid	Isokinetic Sampling, Barium-Thorin Titrimetric Method ^[5]
24	Tin	Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method ^[5]
25	Total Suspended Particulate	1) Isokinetic Sampling, Gravimetric Method ^[5] 2) Paired Train, Isokinetic Sampling, Gravimetric Method ^[5]
26	Vanadium	Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method ^[5]
27	Xylene	1) Adsorption Sampling, Gas Chromatographic Method ^[5] 2) Adsorption Sampling, Gas Chromatographic/Mass Spectrometric Method ^[5]

สิ่งปฏิกูล...

สิ่งปฏิกูลหรือวัสดุที่ไม่ใช้แล้ว จำนวน 34 รายการ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
1	Aldrin	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method ^[1,6,9,22] 2) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[1,6,9,27] 3) Soxhlet Extraction, Gas Chromatographic Method ^[10,22] 4) Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method ^[10,27]
2	Antimony	1) Waste Extraction, Digestion, Hydride Generation/Atomic Absorption Spectrometric Method ^[1,6,16] 2) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[1,6,14] 3) Digestion, Hydride Generation/Atomic Absorption Spectrometric Method ^[7,16] 4) Digestion, Inductively Coupled Plasma Method ^[7,14]
3	Arsenic	1) Waste Extraction, Digestion, Hydride Generation/Atomic Absorption Spectrometric Method ^[1,6,16] 2) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[1,6,14] 3) Digestion, Hydride Generation/Atomic Absorption Spectrometric Method ^[7,16] 4) Digestion, Inductively Coupled Plasma Method ^[7,14]
4	Barium	1) Waste Extraction, Digestion, Flame Atomic Absorption Spectrometric Method ^[1,6,15]

2) Waste Extraction...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
5	Beryllium	2) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[1,6,14] 3) Digestion, Flame Atomic Absorption Spectrometric Method ^[7,15] 4) Digestion, Inductively Coupled Plasma Method ^[7,14]
6	Cadmium	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[1,6,14] 2) Digestion, Inductively Coupled Plasma Method ^[7,14]
7	Chlordane	1) Waste Extraction, Digestion, Flame Atomic Absorption Spectrometric Method ^[1,6,15] 2) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[1,6,14] 3) Digestion, Flame Atomic Absorption Spectrometric Method ^[7,15] 4) Digestion, Inductively Coupled Plasma Method ^[7,14]
8	Chromium	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method ^[1,9,22] 2) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[1,9,27] 3) Soxhlet Extraction, Gas Chromatographic Method ^[10,22] 4) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[10,27] 1) Waste Extraction, Digestion, Flame Atomic Absorption Spectrometric Method ^[1,6,15] 2) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[1,6,14] <i>3) Digestion...</i>

3) Digestion...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
9	Chromium (III)	3) Digestion, Flame Atomic Absorption Spectrometric Method ^[7,15] 4) Digestion, Inductively Coupled Plasma Method ^[7,14] 1) Waste Extraction, Digestion, Flame Atomic Absorption Spectrometric Method; Waste Extraction, Colorimetric Method; Calculation ^[1,6,15,17] 2) Waste Extraction, Digestion, Inductively Coupled Plasma Method; Waste Extraction, Colorimetric Method; Calculation ^[1,6,14,17] 3) Digestion, Flame Atomic Absorption Spectrometric Method; Alkaline Digestion, Colorimetric Method; Calculation ^[7,8,15,17] 4) Digestion, Inductively Coupled Plasma Method; Alkaline Digestion, Colorimetric Method; Calculation ^[7,8,14,17]
10	Chromium (VI)	1) Waste Extraction, Colorimetric Method ^[1,17] 2) Alkaline Digestion, Colorimetric Method ^[8,17]
11	Cobalt	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[1,6,14] 2) Digestion, Inductively Coupled Plasma Method ^[7,14]
12	Copper	1) Waste Extraction, Digestion, Flame Atomic Absorption Spectrometric Method ^[1,6,15] 2) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[1,6,14] 3) Digestion, Flame Atomic Absorption Spectrometric Method ^[7,15] 4) Digestion, Inductively Coupled Plasma Method ^[7,14] <i>3) Digestion...</i>

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
13	2,4-D	1) Waste Extraction, Gas Chromatographic/Mass Spectrometric Method ^[1,25] 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[25]
14	DDD	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method ^[1,9,22] 2) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[1,9,27] 3) Soxhlet Extraction, Gas Chromatographic Method ^[10,22] 4) Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method ^[10,27]
15	DDE	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method ^[1,9,22] 2) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[1,9,27] 3) Soxhlet Extraction, Gas Chromatographic Method ^[10,22] 4) Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method ^[10,27]
16	DDT	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method ^[1,9,22] 2) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[1,9,27] 3) Soxhlet Extraction, Gas Chromatographic Method ^[10,22] 4) Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method ^[10,27] <i>Siman</i>

17 Dieldrin...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
17	Dieldrin	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method ^[1,9,22] 2) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[1,9,27] 3) Soxhlet Extraction, Gas Chromatographic Method ^[10,22] 4) Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method ^[10,27]
18	Endrin	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method ^[1,9,22] 2) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[1,9,27] 3) Soxhlet Extraction, Gas Chromatographic Method ^[10,22] 4) Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method ^[10,27]
19	Heptachlor	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method ^[1,9,22] 2) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[1,9,27] 3) Soxhlet Extraction, Gas Chromatographic Method ^[10,22] 4) Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method ^[10,27]
20	Lead	1) Waste Extraction, Digestion, Flame Atomic Absorption Spectrometric Method ^[1,6,15] 2) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[1,6,14] <i>Siman</i>

3) Digestion...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
21	Lindane	3) Digestion, Flame Atomic Absorption Spectrometric Method ^[7,15] 4) Digestion, Inductively Coupled Plasma Method ^[7,14] 1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method ^[1,9,22] 2) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[1,9,27] 3) Soxhlet Extraction, Gas Chromatographic Method ^[10,22] 4) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[10,27]
22	Mercury	1) Waste Extraction, Digestion, Cold-Vapor Atomic Absorption Spectrometric Method ^[1,18] 2) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[1,6,14] 3) Digestion, Cold-Vapor Atomic Absorption Spectrometric Method ^[19] 4) Digestion, Inductively Coupled Plasma Method ^[7,14]
23	Methoxychlor	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method ^[1,9,22] 2) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[1,9,27] 3) Soxhlet Extraction, Gas Chromatographic Method ^[10,22] 4) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[10,27]


24 Molybdenum...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
24	Molybdenum	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[1,6,14] 2) Digestion, Inductively Coupled Plasma Method ^[7,14]
25	Nickel	1) Waste Extraction, Digestion, Flame Atomic Absorption Spectrometric Method ^[1,6,15] 2) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[1,6,14] 3) Digestion, Flame Atomic Absorption Spectrometric Method ^[7,15] 4) Digestion, Inductively Coupled Plasma Method ^[7,14]
26	Polychlorinated Biphenyls - Aroclor 1016 - Aroclor 1221 - Aroclor 1232 - Aroclor 1242 - Aroclor 1248 - Aroclor 1254 - Aroclor 1260	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method ^[1,9,23] 2) Soxhlet Extraction, Gas Chromatographic Method ^[10,23]
27	Pentachlorophenol	1) Waste Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[1,25] 2) Ultrasonic Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[25]
28	pH	Electrometric Method ^[31,32]
29	Selenium	1) Waste Extraction, Digestion, Hydride Generation/Atomic Absorption Spectrometric Method ^[1,6,20] 2) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[1,6,14] 3) Digestion, Hydride Generation/Atomic Absorption Spectrometric Method ^[7,20]


4) Digestion...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
30	Silver	4) Digestion, Inductively Coupled Plasma Method ^[7,14] 1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[1,6,14] 2) Digestion, Inductively Coupled Plasma Method ^[7,14]
31	Thallium	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[1,6,14] 2) Digestion, Inductively Coupled Plasma Method ^[7,14]
32	Trichloroethylene	1) Waste Extraction, Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[1,12,26] 2) Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[12,26]
33	Vanadium	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[1,6,14] 2) Digestion, Inductively Coupled Plasma Method ^[7,14]
34	Zinc	1) Waste Extraction, Digestion, Flame Atomic Absorption Spectrometric Method ^[1,6,15] 2) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[1,6,14] 3) Digestion, Flame Atomic Absorption Spectrometric Method ^[7,15] 4) Digestion, Inductively Coupled Plasma Method ^[7,14]

ดิน จำนวน 124 รายการ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
1	Acenaphthene	Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method ^[10,27] 

2 Acetone...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
2	Acetone	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[13,26]
3	Aldrin	1) Ultrasonic Extraction, Gas Chromatographic Method ^[11,22] 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[11,27]
4	Anthracene	Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method ^[10,27]
5	Antimony	1) Digestion, Hydride Generation/Atomic Absorption Spectrometric Method ^[7,16] 2) Digestion, Inductively Coupled Plasma Method ^[7,14]
6	Arsenic	1) Digestion, Hydride Generation/Atomic Absorption Spectrometric Method ^[7,16] 2) Digestion, Inductively Coupled Plasma Method ^[7,14]
7	Atrazine	Ultrasonic Extraction, Gas Chromatographic Method ^[11,24]
8	Barium	1) Digestion, Flame Atomic Absorption Spectrometric Method ^[7,15] 2) Digestion, Inductively Coupled Plasma Method ^[7,14]
9	Benz(a)anthracene	Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method ^[10,27]
10	Benzene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[13,26]
11	Benzo(b)fluoranthene	Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method ^[10,27]
12	Benzo(k)fluoranthene	Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method ^[10,27]
13	Benzoic acid	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[11,27] 

14 Benzo(a)pyrene...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
14	Benzo(a)pyrene	Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[10,27]
15	Benzo(g,h,i)perylene	Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[10,27]
16	Beryllium	Digestion, Inductively Coupled Plasma Method ^[7,14]
17	Bis(2-chloroethyl)ether	Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[10,27]
18	Bis(2-ethylhexyl)phthalate	Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[10,27]
19	Bromodichloromethane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[13,26]
20	Bromoform	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[13,26]
21	Butanol	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[13,26]
22	Butyl benzyl phthalate	Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[10,27]
23	Cadmium	1) Digestion, Flame Atomic Absorption Spectrometric Method ^[7,15] 2) Digestion, Inductively Coupled Plasma Method ^[7,14]
24	Carbazole	Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[10,27]
25	Carbon disulfide	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[13,26]
26	Carbon tetrachloride	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[13,26]
27	Chlordane	1) Ultrasonic Extraction, Gas Chromatographic Method ^[11,22] 2) Ultrasonic Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[11,27]


ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
28	p-Chloroaniline	Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[10,27]
29	Chlorobenzene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[13,26]
30	Chlorodibromomethane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[13,26]
31	Chloroform	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[13,26]
32	2-Chlorophenol	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[11,27]
33	Chromium	1) Digestion, Flame Atomic Absorption Spectrometric Method ^[7,15] 2) Digestion, Inductively Coupled Plasma Method ^[7,14]
34	Chromium (III)	1) Digestion, Flame Atomic Absorption Spectrometric Method; Colorimetric Method; Calculation ^[7,8,15,17] 2) Digestion, Inductively Coupled Plasma Method; Colorimetric Method; Calculation ^[7,8,14,17]
35	Chromium (VI)	Alkaline Digestion, Colorimetric Method ^[8,17]
36	Chrysene	Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[10,27]
37	Cyanide	1) Extraction, Distillation, Titrimetric Method ^[28,29,30] 2) Extraction, Distillation, Colorimetric Method ^[28,29,30]
38	2,4-D	Ultrasonic Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[24]
39	DDD	1) Ultrasonic Extraction, Gas Chromatographic Method ^[11,22] 2) Ultrasonic Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[11,27]

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
40	DDE	1) Ultrasonic Extraction, Gas Chromatographic Method ^[11,22] 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[11,27]
41	DDT	1) Ultrasonic Extraction, Gas Chromatographic Method ^[11,22] 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[11,27]
42	Dibenz(a,h)anthracene	Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method ^[10,27]
43	Di-n-butyl phthalate	Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method ^[10,27]
44	1,2-Dichlorobenzene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[13,26]
45	1,3-Dichlorobenzene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[13,26]
46	1,4-Dichlorobenzene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[13,26]
47	3,3'-Dichlorobenzidine	Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method ^[10,27]
48	1,1-Dichloroethane	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[13,26]
49	1,2-Dichloroethane	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[13,26]
50	1,1-Dichloroethylene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[13,26]
51	cis-1,2-Dichloroethylene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[13,26]
52	trans-1,2-Dichloroethylene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[13,26]
53	2,4-Dichlorophenol	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[11,27]


54 1,2-Dichloropropane...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
54	1,2-Dichloropropane	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[13,26]
55	1,3-Dichloropropane	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[13,26]
56	1,3-Dichloropropene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[13,26]
57	Dieldrin	1) Ultrasonic Extraction, Gas Chromatographic Method ^[11,22] 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[11,27]
58	Diethyl phthalate	Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method ^[10,27]
59	2,4-Dimethylphenol	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[11,27]
60	2,4-Dinitrophenol	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[11,27]
61	2,4-Dinitrotoluene	Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method ^[10,27]
62	2,6-Dinitrotoluene	Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method ^[10,27]
63	Di-n-Octyl phthalate	Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method ^[10,27]
64	Endosulfan	1) Ultrasonic Extraction, Gas Chromatographic Method ^[11,22] 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[11,27]
65	Endrin	1) Ultrasonic Extraction, Gas Chromatographic Method ^[11,22] 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[11,27]
66	Ethylbenzene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[13,26]

67 Fluoranthene...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
67	Fluoranthene	Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[10,27]
68	Fluorene	Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[10,27]
69	Heptachlor	1) Ultrasonic Extraction, Gas Chromatographic Method ^[11,22] 2) Ultrasonic Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[11,27]
70	Heptachlor epoxide	1) Ultrasonic Extraction, Gas Chromatographic Method ^[11,22] 2) Ultrasonic Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[11,27]
71	Hexachlorobenzene	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[11,27]
72	Hexachloro-1,3-butadiene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[13,26]
73	n-Hexane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[13,26]
74	α-HCH	1) Ultrasonic Extraction, Gas Chromatographic Method ^[11,22] 2) Ultrasonic Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[11,27]
75	β-HCH	1) Ultrasonic Extraction, Gas Chromatographic Method ^[11,22] 2) Ultrasonic Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[11,27]
76	γ-HCH	1) Ultrasonic Extraction, Gas Chromatographic Method ^[11,22] 2) Ultrasonic Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[11,27]
77	Hexachlorocyclopentadiene	Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method ^[10,27] 

78 Hexachloroethane...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
78	Hexachloroethane	Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method ^[10,27]
79	Indeno(1,2,3-cd)pyrene	Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method ^[10,27]
80	Isophorone	Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method ^[10,27]
81	Lead	1) Digestion, Flame Atomic Absorption Spectrometric Method ^[7,15] 2) Digestion, Inductively Coupled Plasma Method ^[7,14]
82	Manganese	1) Digestion, Flame Atomic Absorption Spectrometric Method ^[7,15] 2) Digestion, Inductively Coupled Plasma Method ^[7,14]
83	Mercury	1) Digestion, Cold-Vapor Atomic Absorption Spectrometric Method ^[19] 2) Digestion, Inductively Coupled Plasma Method ^[7,14]
84	Methanol	Ultrasonic Extraction, Direct Aqueous Injection, Gas Chromatographic Method ^[11,21]
85	Methoxychlor	1) Ultrasonic Extraction, Gas Chromatographic Method ^[11,22] 2) Ultrasonic Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[11,27]
86	Methyl bromide	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[13,26]
87	Methylene chloride	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[13,26]
88	2-Methylphenol	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[11,27]
89	2-Methylnaphthalene	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[11,27] 

90 Methyl tert-butyl ether...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
90	Methyl tert-butyl ether	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[13,26]
91	Naphthalene	Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method ^[10,27]
92	Nickel	1) Digestion, Flame Atomic Absorption Spectrometric Method ^[7,15] 2) Digestion, Inductively Coupled Plasma Method ^[7,14]
93	Nitrobenzene	Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method ^[10,27]
94	N-Nitrosodiphenylamine	Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method ^[10,27]
95	N-Nitrosodi-n-propylamine	Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method ^[10,27]
96	Polychlorinated Biphenyls - Aroclor 1016 - Aroclor 1221 - Aroclor 1232 - Aroclor 1242 - Aroclor 1248 - Aroclor 1254 - Aroclor 1260	Soxhlet Extraction, Gas Chromatographic Method ^[10,23]
97	Pentachlorophenol	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[24]
98	Phenanthrene	Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method ^[10,27]
99	Phenol	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[11,27]
100	Pyrene	Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method ^[10,27]
101	Selenium	1) Digestion, Hydride Generation/Atomic Absorption Spectrometric Method ^[7,20]

2) Digestion...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
102	Silver	2) Digestion, Inductively Coupled Plasma Method ^[7,14] 1) Digestion, Flame Atomic Absorption Spectrometric Method ^[7,15] 2) Digestion, Inductively Coupled Plasma Method ^[7,14]
103	Styrene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[13,26]
104	1,1,2,2-Tetrachloroethane	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[13,26]
105	Tetrachloroethylene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[13,26]
106	Toluene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[13,26]
107	TPH (C ₅ -C ₈)	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[13,26]
108	TPH (C ₈ -C ₁₆)	1) Soxhlet Extraction, Gas Chromatographic Method ^[10,21] 2) Soxhlet Extraction, Gas Chromatographic/Mass spectrometric Method ^[10,26]
109	TPH (C ₁₆ -C ₃₅)	1) Soxhlet Extraction, Gas Chromatographic Method ^[10,21] 2) Soxhlet Extraction, Gas Chromatographic/Mass spectrometric Method ^[10,26]
110	1,2,4-Trichlorobenzene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[13,26]
111	1,1,1-Trichloroethane	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[13,26]
112	1,1,2-Trichloroethane	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[13,26]
113	Trichloroethylene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[13,26]

114 2,4,5-Trichlorophenol...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
114	2,4,5-Trichlorophenol	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[11,27]
115	2,4,6-Trichlorophenol	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[11,27]
116	1,3,5-Trimethylbenzene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[13,26]
117	Vanadium	Digestion, Inductively Coupled Plasma Method ^[7,14]
118	Vinyl acetate	Purge and Trap, Gas Chromatographic/Mass spectrometric Method ^[13,26]
119	Vinyl chloride	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[13,26]
120	m-Xylene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[13,26]
121	o-Xylene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[13,26]
122	p-Xylene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[13,26]
123	Xylene (Total)	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[13,26]
124	Zinc	1) Digestion, Flame Atomic Absorption Spectrometric Method ^[7,15] 2) Digestion, Inductively Coupled Plasma Method ^[7,14]

เอกสารอ้างอิง

- กระทรวงอุตสาหกรรม. ประกาศกระทรวงอุตสาหกรรม, พ.ศ. 2548. เรื่อง การกำจัดสิ่งปฏิกูลหรือวัสดุที่ไม่ใช้แล้ว.ราชกิจจานุเบกษา. 25 มกราคม 2549. เล่มที่ 123 ตอนพิเศษ 11ง.
- กระทรวงอุตสาหกรรม. ประกาศกระทรวงอุตสาหกรรม, พ.ศ. 2549. เรื่อง กำหนดค่าปริมาณเขม่าควันที่เจือปนในอากาศที่ระบายออกจากปล่องของหม้อน้ำโรงสีข้าวที่ใช้กลบเป็นเชื้อเพลิง.ราชกิจจานุเบกษา. 4 ธันวาคม 2549. เล่มที่ 123 ตอนพิเศษ 125ง.
- สมาคมวิศวกรรมสิ่งแวดล้อมแห่งประเทศไทย. คู่มือวิเคราะห์น้ำเสีย. พิมพ์ครั้งที่ 4. กรุงเทพฯ: เรือนแก้วการพิมพ์, 2547.

4. APHA, AWWA, WEF. **Standard Methods for the Examination of Water and Wastewater**. 23rd ed. Washington, DC: APHA, 2017.
5. United States Environmental Protection Agency. **Standards of Performance for New Stationary Sources**. 40 CFR 60. Appendix A, 2023.
6. United States Environmental Protection Agency. **Test Methods for Evaluation Solid Waste Physical/Chemical Methods**. SW-846, 2020.
7. United States Environmental Protection Agency. **Test Methods for Evaluation Solid Waste Physical/Chemical Methods**. **Acid Digestion of Sediments, Sludges, and Soils**. SW-846 Method 3050B, 1996.
8. United States Environmental Protection Agency. **Test Methods for Evaluation Solid Waste Physical/Chemical Methods**. **Alkaline Digestion for Hexavalent Chromium**. SW-846 Method 3060A, 1996.
9. United States Environmental Protection Agency. **Test Methods for Evaluation Solid Waste Physical/Chemical Methods**. **Separatory Funnel Liquid-Liquid Extraction**. SW-846 Method 3510C, 1996.
10. United States Environmental Protection Agency. **Test Methods for Evaluation Solid Waste Physical/Chemical Methods**. **Soxhlet Extraction**. SW-846 Method 3540C, 1996.
11. United States Environmental Protection Agency. **Test Methods for Evaluation Solid Waste Physical/Chemical Methods**. **Ultrasonic Extraction**. SW-846 Method 3550C, 2007.
12. United States Environmental Protection Agency. **Test Methods for Evaluation Solid Waste Physical/Chemical Methods**. **Purge-and-Trap for Aqueous Samples**. SW-846 Method 5030C, 2003.
13. United States Environmental Protection Agency. **Test Methods for Evaluation Solid Waste Physical/Chemical Methods**. **Closed-System Purge-and-Trap and Extraction for Volatile Organics in Soil and Waste Samples**. SW-846 Method 5035, 1996.
14. United States Environmental Protection Agency. **Test Methods for Evaluation Solid Waste Physical/Chemical Methods**. **Inductively Coupled Plasma-optical Emission Spectrometry**. SW-846 Method 6010D, 2018.
15. United States Environmental Protection Agency. **Test Methods for Evaluation Solid Waste Physical/Chemical Methods**. **Flame Atomic Absorption Spectrophotometry**. SW-846 Method 7000B, 2007.
16. United States Environmental Protection Agency. **Test Methods for Evaluation Solid Waste Physical/Chemical Methods**. **Antimony and Arsenic (Atomic Absorption, Borohydride Reduction)**. SW-846 Method 7062, 1994.

17. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Chromium, Hexavalent (Colorimetric), SW-846 Method 7196A**, 1992.

18. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Mercury in Liquid Waste (Manual Cold-Vapor Technique, SW-846 Method 7470A**, 1994.

19. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Mercury in Solid or Semisolid Waste (Manual Cold-Vapor Technique, SW-846 Method 7471B**, 2007.

20. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Selenium (Atomic Absorption, Borohydride Reduction), SW-846 Method 7742**, 1994.

21. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Nonhalogenated Organics Using GC/FID. SW-846 Method 8015D**, 2003.

22. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Organochlorine Pesticide by Gas Chromatography. SW-846 Method 8081B**, 2007.

23. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Polychlorinated Biphenyls (PCBs) By Gas Chromatography. SW-846 Method 8082A**, 2007.

24. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Organophosphorus Compounds by Gas Chromatography. SW-846 Method 8141B**, 2007.

25. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Chlorinated Herbicides By GC Using Methylation or Pentafluorobenzoylation Derivatization. SW-846 Method 8151A**, 1996.

26. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Volatile Organic Compounds by Gas Chromatography/ Mass Spectrometry (GC/MS). SW-846 Method 8260D**, 2018.

27. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **SemiVolatile Organic Compounds by Gas Chromatography/Mass Spectrometry. SW-846 Method 8270E**, 2018. 

28. United States...

28. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Total and Amenable Cyanide: Distillation. SW-846 Method 9010C**, 2004.

29. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Cyanide Extraction Procedure for Solids and Oils. SW-846 Method 9013A**, 2014.

30. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Cyanide in Waters and Extracts Using Titrimetric and Manual Spectrophotometric. SW-846 Method 9014**, 2014.

31. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **pH Electrometric Measurement. SW-846 Method 9040C**, 2004.

32. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Solid and Waste pH. SW-846 Method 9045D**, 2004. 

ที่ ออก ๐๓๑๐(๑)/ ๕๐ ๕๕



กรมโรงงานอุตสาหกรรม
ถนนพระรามที่ ๖ แขวงทุ่งพญาไท
เขตราชเทวี กรุงเทพฯ ๑๐๔๐๐

๒๗ พฤษภาคม ๒๕๖๗

เรื่อง เปลี่ยนแปลงบุคลากรของห้องปฏิบัติการวิเคราะห์

เรียน กรรมการผู้จัดการ บริษัท ซิคอท จำกัด

อ้างถึง คำขอขึ้นทะเบียน/ต่ออายุ/เปลี่ยนแปลงบุคลากร และชนิดสารมลพิษของห้องปฏิบัติการวิเคราะห์เอกชน
ลงวันที่ ๒๑ พฤษภาคม ๒๕๖๗

ตามคำขอที่อ้างถึง บริษัท ซิคอท จำกัด ห้องปฏิบัติการวิเคราะห์เอกชน เลขทะเบียน ว-๒๓๙
สถานที่ตั้งเลขที่ ๒๓๙ ถนนริมคลองประปา แขวงบางซื่อ เขตบางซื่อ กรุงเทพมหานคร ขอเปลี่ยนแปลงบุคลากร
ความละเอียดแจ้งแล้ว นั้น

กรมโรงงานอุตสาหกรรมพิจารณาแล้ว ให้ยกเลิกเจ้าหน้าที่ประจำห้องปฏิบัติการวิเคราะห์
จำนวน ๒ ราย ได้แก่

๑) นายวัชรกานต์ ประมาคะเต

ทะเบียนเลขที่ ว-๒๓๙-จ-๐๐๑๕

๒) นายรัตนชัย ขอบทำกิจ

ทะเบียนเลขที่ ว-๒๓๙-จ-๐๐๓๐

จึงเรียนมาเพื่อทราบ

ขอแสดงความนับถือ


(นายพรศ กลั่นกรอง)
รองอธิบดี ปฏิบัติราชการแทน
อธิบดีกรมโรงงานอุตสาหกรรม

กองวิจัยและเตือนภัยมลพิษโรงงาน

กลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษและทะเบียนห้องปฏิบัติการ

โทร. ๐ ๒๔๓๐ ๖๓๑๒ ต่อ ๒๑๐๓-๕

โทรสาร ๐ ๒๔๓๐ ๖๓๑๒ ต่อ ๒๑๔๔

ไปรษณีย์อิเล็กทรอนิกส์ saraban@diw.mail.go.th



ที่ ออก ๐๓๑๐(๑)/ ๑๑ ๕๕ ๗



กรมโรงงานอุตสาหกรรม
ถนนพระรามที่ ๖ แขวงทุ่งพญาไท
เขตราชเทวี กรุงเทพฯ ๑๐๔๐๐

๒๑ พฤศจิกายน ๒๕๖๗

เรื่อง ยกเลิกบุคลากรของห้องปฏิบัติการวิเคราะห์

เรียน กรรมการผู้จัดการ บริษัท ซิคอท จำกัด

อ้างถึง คำขอขึ้นทะเบียน/ต่ออายุ/เปลี่ยนแปลงบุคลากร และชนิดสารมลพิษของห้องปฏิบัติการวิเคราะห์เอกชน
ลงวันที่ ๕ พฤศจิกายน ๒๕๖๗

ตามคำขอที่อ้างถึง บริษัท ซิคอท จำกัด ห้องปฏิบัติการวิเคราะห์เอกชน เลขทะเบียน ว-๒๓๙
สถานที่ตั้งเลขที่ ๒๓๙ ถนนริมคลองประปา แขวงบางซื่อ เขตบางซื่อ กรุงเทพมหานคร ขอยกเลิกบุคลากร
ความละเอียดแจ้งแล้ว นั้น

กรมโรงงานอุตสาหกรรมพิจารณาแล้ว ให้ยกเลิกเจ้าหน้าที่ประจำห้องปฏิบัติการวิเคราะห์
จำนวน ๓ ราย ได้แก่

๑) นางสาวพัชรา สมานฉันท์

ทะเบียนเลขที่ ว-๒๓๙-จ-๐๐๒๑

๒) นางสาวสุภาวดี บัวแก้ว


ทะเบียนเลขที่ ว-๒๓๙-จ-๐๐๓๖

๓) นางสาวมาริยามณี ฮาแว

ทะเบียนเลขที่ ว-๒๓๙-จ-๐๐๓๗

จึงเรียนมาเพื่อทราบ

ขอแสดงความนับถือ


(นายธีรทัศน์ อิศรางกูร ณ อยุธยา)
รองอธิบดี ปฏิบัติราชการแทน
อธิบดีกรมโรงงานอุตสาหกรรม

กองวิจัยและเตือนภัยมลพิษโรงงาน

กลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษและทะเบียนห้องปฏิบัติการ

โทร. ๐ ๒๔๓๐ ๖๓๑๒ ต่อ ๒๑๐๓-๕

โทรสาร ๐ ๒๔๓๐ ๖๓๑๒ ต่อ ๒๑๔๔

ไปรษณีย์อิเล็กทรอนิกส์ saraban@diw.mail.go.th



ภาคผนวก ช

ใบรับรองความสามารถห้องปฏิบัติการและขอบข่ายการรับรอง
(Certification of Laboratory Accreditation)



แบบ กมช./สมอ.๒
Form NSC/TISI 2

ใบรับรองเลขที่ 24-LB0026
(Certificate No.)

ใบรับรองระบบงาน

(Certificate of Accreditation)

อาศัยอำนาจตามความในพระราชบัญญัติการมาตรฐานแห่งชาติ พ.ศ. ๒๕๕๑
(By Virtue of National Standardization Act B.E. 2551 (2008))

เลขาธิการสำนักงานมาตรฐานผลิตภัณฑ์อุตสาหกรรม
(Secretary-General, Thai Industrial Standards Institute)

ออกใบรับรองฉบับนี้ให้

(Issues this certificate to)

บริษัท ซีคोट จำกัด ฝ่ายห้องปฏิบัติการทดสอบด้านสิ่งแวดล้อม
(Secot Company Limited, Environmental Laboratory Division)

ตั้งอยู่เลขที่
(Address)

๒๓๙ ถนนริมคลองประปา แขวงบางซื่อ เขตบางซื่อ กรุงเทพมหานคร
(239 Rimklongprapa Road, Bangsue, Bangkok)

ได้รับการรับรองความสามารถ

(Certificate of competence)

ตามมาตรฐานเลขที่ มอก. ๑๗๐๒๕ - ๒๕๖๑
(Standard No. TIS 17025-2561 (2018) (ISO/IEC 17025: 2017))

ข้อกำหนดทั่วไปว่าด้วยความสามารถของ ห้องปฏิบัติการทดสอบและห้องปฏิบัติการสอบเทียบ
(General requirements for the competence of testing and calibration laboratories)

หมายเลขการรับรองที่ ทดสอบ ๐๓๙๔
(Accreditation No. Testing 0394)

โดยมีรายละเอียดสาขาและขอบข่ายที่ใบรับรอง แสดงไว้ใน QR CODE และ www.tisi.go.th
(Details of the scheme and scope of the certificate are shown in QR CODE and www.tisi.go.th)

ออกให้ ณ วันที่ ๖ ธันวาคม พ.ศ. ๒๕๖๖
(Issue date : 6 December B.E. 2566 (2023))

(นายวีระศักดิ์ เพ็งหล่ง)

ผู้อำนวยการสำนักงานคณะกรรมการการมาตรฐานแห่งชาติ
ปฏิบัติราชการแทน

เลขาธิการสำนักงานมาตรฐานผลิตภัณฑ์อุตสาหกรรม



Signed by สำนักงานมาตรฐานผลิตภัณฑ์อุตสาหกรรม (สมอ.)
Thai Industrial Standards Institute (TISI)
Date: 2023-12-06T08:49:04.476+07:00

d68cb66b

กระทรวงอุตสาหกรรม สำนักงานมาตรฐานผลิตภัณฑ์อุตสาหกรรม
(Ministry of Industry Thailand, Thai Industrial Standards Institute)



รายละเอียดสาขาและขอบข่ายใบรับรองห้องปฏิบัติการ
(Scope of Accreditation for Testing)
ใบรับรองเลขที่ 24-LB0026
(Certification No. 24-LB0026)



ชื่อห้องปฏิบัติการ
(Laboratory Name)

บริษัท ซีคोट จำกัด ฝ่ายห้องปฏิบัติการทดสอบด้านสิ่งแวดล้อม
(Secot Company Limited, Environmental Laboratory Division)

หมายเลขการรับรองที่
(Accreditation No.)

ทดสอบ 0394
(Testing 0394)

ฉบับที่ 02
(Issue No.02)

ออกให้ตั้งแต่วันที่ 30 ตุลาคม พ.ศ. 2566
(Valid from) (30 October B.E.2566 (2023))

ถึงวันที่ 8 กันยายน พ.ศ. 2571
(Until) (8 September B.E.2571 (2028))

สถานภาพห้องปฏิบัติการ
(Laboratory status)

☒ถาวร
(Permanent)

☐นอกสถานที่
(Site)

☐ชั่วคราว
(Temporary)

☐เคลื่อนที่
(Mobile)

☐หลายสถานที่
(Multisite)

สาขาการทดสอบ (Field of Testing)	รายการทดสอบ (Parameter)	วิธีทดสอบ (Test Method)
สาขาสังแวดล้อม (environmental field) 1. น้ำและน้ำเสีย (water and wastewater)	- โลหะหนัก (heavy metals) • สารหนู (Arsenic, As) 0.000 5 mg/L ถึง 0.090 0 mg/L • สารหนู (Arsenic, As) 0.05 mg/L ถึง 4.50 mg/L • แบเรียม (Barium, Ba) 0.02 mg/L ถึง 4.50 mg/L • แคดเมียม (Cadmium, Cd) 0.01 mg/L ถึง 4.50 mg/L • โครเมียม (Chromium, Cr) 0.01 mg/L ถึง 4.50 mg/L	- Standard Methods for the Examination of Water and Wastewater, APHA, AWWA, WEF, 23 rd edition, 2017, Part 3030 F and Part 3114 C - Standard Methods for the Examination of Water and Wastewater, APHA, AWWA, WEF, 23 rd edition, 2017, Part 3030 E and Part 3120 B

กระทรวงอุตสาหกรรม สำนักงานมาตรฐานผลิตภัณฑ์อุตสาหกรรม
(Ministry of Industry, Thai Industrial Standards Institute)

หน้าที่ 1/9

รายละเอียดสาขาและขอบข่ายใบรับรองห้องปฏิบัติการ

(Scope of Accreditation for Testing)

ใบรับรองเลขที่ 24-LB0026

(Certification No. 24-LB0026)



ฉบับที่ 02
(Issue No.02)

ออกให้ตั้งแต่วันที่ 30 ตุลาคม พ.ศ. 2566
(Valid from) (30 October B.E.2566 (2023))

ถึงวันที่ 8 กันยายน พ.ศ. 2571
(Until) (8 September B.E.2571 (2028))

สถานภาพห้องปฏิบัติการ
(Laboratory status)

☒ถาวร
(Permanent)

☐นอกสถานที่
(Site)

☐ชั่วคราว
(Temporary)

☐เคลื่อนที่
(Mobile)

☐หลายสถานที่
(Multisite)

สาขาการทดสอบ (Field of Testing)	รายการทดสอบ (Parameter)	วิธีทดสอบ (Test Method)
<p>สาขาสสิ่งแวดล้อม (environmental field)</p> <p>1. น้ำและน้ำเสีย (ต่อ) (water and wastewater) (cont.)</p>	<p>- โลหะหนัก (heavy metals)</p> <ul style="list-style-type: none"> ทองแดง (Copper, Cu) 0.02 mg/L ถึง 4.50 mg/L เหล็ก (Iron, Fe) 0.05 mg/L ถึง 9.00 mg/L ตะกั่ว (Lead, Pb) 0.03 mg/L ถึง 4.50 mg/L แมงกานีส (Manganese, Mn) 0.01 mg/L ถึง 9.00 mg/L นิกเกิล (Nickel, Ni) 0.01 mg/L ถึง 4.50 mg/L สังกะสี (Zinc, Zn) 0.02 mg/L ถึง 9.00 mg/L 	<p>- Standard Methods for the Examination of Water and Wastewater, APHA , AWWA, WEF, 23rd edition , 2017, Part 3030 E and Part 3120 B</p>

รายละเอียดสาขาและขอบข่ายใบรับรองห้องปฏิบัติการ

(Scope of Accreditation for Testing)

ใบรับรองเลขที่ 24-LB0026

(Certification No. 24-LB0026)



ฉบับที่ 02
(Issue No.02)

ออกให้ตั้งแต่วันที่ 30 ตุลาคม พ.ศ. 2566
(Valid from) (30 October B.E.2566 (2023))

ถึงวันที่ 8 กันยายน พ.ศ. 2571
(Until) (8 September B.E.2571 (2028))

สถานภาพห้องปฏิบัติการ
(Laboratory status)

☒ถาวร
(Permanent)

☐นอกสถานที่
(Site)

☐ชั่วคราว
(Temporary)

☐เคลื่อนที่
(Mobile)

☐หลายสถานที่
(Multisite)

สาขาการทดสอบ (Field of Testing)	รายการทดสอบ (Parameter)	วิธีทดสอบ (Test Method)
<p>สาขาสสิ่งแวดล้อม (environmental field)</p> <p>1. น้ำและน้ำเสีย (ต่อ) (water and wastewater) (cont.)</p>	<p>- ซีโอดี (Chemical oxygen demand, COD) 100 mg/L ถึง 4 000 mg/L</p>	<p>- Standard Methods for the Examination of Water and Wastewater, APHA, AWWA, WEF, 23rd edition , 2017, Part 5220 D</p>
<p>2. บริเวณทำงาน (workplace)</p>	<p>- ฝุ่นละอองรวม (Total dust) 0.10 mg/filter ถึง 2.00 mg/filter</p> <p>- ฝุ่นละอองขนาดเล็ก (Respirable dust) 0.10 mg/filter ถึง 2.00 mg/filter</p>	<p>- NIOSH Manual of Analytical Methods (NMAM) , method 0500, 4th edition , 15th August 1994 (Exclude Sampling)</p> <p>- NIOSH Manual of Analytical Methods (NMAM) , method 0600, 4th edition , 15th January 1998 (Exclude Sampling)</p>

รายละเอียดสาขาและขอบข่ายใบรับรองห้องปฏิบัติการ
(Scope of Accreditation for Testing)

ใบรับรองเลขที่ 24-LB0026
(Certification No. 24-LB0026)



ฉบับที่ 02
(Issue No.02)

ออกให้ตั้งแต่วันที่ 30 ตุลาคม พ.ศ. 2566
(Valid from) (30 October B.E.2566 (2023))

ถึงวันที่ 8 กันยายน พ.ศ. 2571
(Until) (8 September B.E.2571 (2028))

สถานภาพห้องปฏิบัติการ
(Laboratory status)

☒ถาวร
(Permanent)

☐นอกสถานที่
(Site)

☐ชั่วคราว
(Temporary)

☐เคลื่อนที่
(Mobile)

☐หลายสถานที่
(Multisite)

สาขาการทดสอบ (Field of Testing)	รายการทดสอบ (Parameter)	วิธีทดสอบ (Test Method)
<p>สาขาส่งแวดล้อม (environmental field)</p> <p>2. บริเวณทำงาน (ต่อ) (workplace) (cont.)</p>	<ul style="list-style-type: none"> เบนซีน (Benzene) 1.10 µg/tube ถึง 420 µg/tube โทลูอีน (Toluene) 1.10 µg/tube ถึง 420 µg/tube โทโครไซลีน (Total xylenes) 2.20 µg/tube ถึง 840 µg/tube เมตา, พารา-ไซลีน (m, p- Xylene) 1.10 µg/tube ถึง 420 µg/tube ออร์โธ-ไซลีน (o- Xylene) 1.10 µg/tube ถึง 420 µg/tube 	<ul style="list-style-type: none"> NIOSH Manual of Analytical Methods (NMAM) , method 1501, 4th edition , 15th March 2003 (Exclude Sampling)
<p>3. ปล่องระบายอากาศ (stack)</p>	<ul style="list-style-type: none"> ซัลเฟอร์ไดออกไซด์ (Sulfur dioxide) 1.00 mg/L ถึง 16 000 mg/L (solution) 	<ul style="list-style-type: none"> US.EPA , Code of Federal Regulations , 40 CFR 60 appendix A , method 6 , July 2019 (Exclude Sampling)

รายละเอียดสาขาและขอบข่ายใบรับรองห้องปฏิบัติการ
(Scope of Accreditation for Testing)

ใบรับรองเลขที่ 24-LB0026
(Certification No. 24-LB0026)



ฉบับที่ 02
(Issue No.02)

ออกให้ตั้งแต่วันที่ 30 ตุลาคม พ.ศ. 2566
(Valid from) (30 October B.E.2566 (2023))

ถึงวันที่ 8 กันยายน พ.ศ. 2571
(Until) (8 September B.E.2571 (2028))

สถานภาพห้องปฏิบัติการ
(Laboratory status)

☒ถาวร
(Permanent)

☐นอกสถานที่
(Site)

☐ชั่วคราว
(Temporary)

☐เคลื่อนที่
(Mobile)

☐หลายสถานที่
(Multisite)

สาขาการทดสอบ (Field of Testing)	รายการทดสอบ (Parameter)	วิธีทดสอบ (Test Method)
<p>สาขาส่งแวดล้อม (environmental field)</p> <p>3. ปล่องระบายอากาศ (ต่อ) (stack) (cont.)</p>	<ul style="list-style-type: none"> ไฮโดรเจนฟลูออไรด์ (Hydrogen fluoride) 5 µg/sample ถึง 400 µg/sample ไฮโดรเจนคลอไรด์ (Hydrogen chloride) 5 µg/sample ถึง 400 µg/sample 	<ul style="list-style-type: none"> WI-7.2-1-22 based on US.EPA , Code of Federal Regulations , 40 CFR 60 appendix A, method 26 , 2019 (Exclude Sampling)

รายละเอียดสาขาและขอบข่ายใบรับรองห้องปฏิบัติการ
(Scope of Accreditation for Testing)

ใบรับรองเลขที่ 24-LB0026
(Certification No. 24-LB0026)



ฉบับที่ 02
(Issue No.02)

ออกให้ตั้งแต่วันที่ 30 ตุลาคม พ.ศ. 2566
(Valid from) (30 October B.E.2566 (2023))

ถึงวันที่ 8 กันยายน พ.ศ. 2571
(Until) (8 September B.E.2571 (2028))

สถานภาพห้องปฏิบัติการ
(Laboratory status)

☒ถาวร
(Permanent)

☒นอกสถานที่
(Site)

☐ชั่วคราว
(Temporary)

☐เคลื่อนที่
(Mobile)

☐หลายสถานที่
(Multisite)

สาขาการทดสอบ (Field of Testing)	รายการทดสอบ (Parameter)	วิธีทดสอบ (Test Method)
<p>สาขาสสิ่งแวดล้อม (environmental field)</p> <p>4. บรรยากาศทั่วไป (ambient air)</p>	<p>- สารอินทรีย์ระเหยง่าย (Volatile organic compounds, VOCs)</p> <ul style="list-style-type: none"> คลอโรอีthin (Chloroethene) 0.05 $\mu\text{g}/\text{m}^3$ ถึง 51.00 $\mu\text{g}/\text{m}^3$ (0.02 ppbv ถึง 20.00 ppbv) 1,3-บิวทาไดเอิน (1,3-butadiene) 0.04 $\mu\text{g}/\text{m}^3$ ถึง 44.00 $\mu\text{g}/\text{m}^3$ (0.02 ppbv ถึง 20.00 ppbv) โบรมอมีเทน (Bromomethane) 0.08 $\mu\text{g}/\text{m}^3$ ถึง 77.00 $\mu\text{g}/\text{m}^3$ (0.02 ppbv ถึง 20.00 ppbv) อะคลอลีน (Acrolein) 0.05 $\mu\text{g}/\text{m}^3$ ถึง 45.00 $\mu\text{g}/\text{m}^3$ (0.02 ppbv ถึง 20.00 ppbv) 	<p>- WI-7.2-1-24 based on US EPA , Compendium Method TO-15 , EPA/625/R-96/010b, Second edition, January 1999</p> <p><i>W</i></p>

รายละเอียดสาขาและขอบข่ายใบรับรองห้องปฏิบัติการ
(Scope of Accreditation for Testing)

ใบรับรองเลขที่ 24-LB0026
(Certification No. 24-LB0026)



ฉบับที่ 02
(Issue No.02)

ออกให้ตั้งแต่วันที่ 30 ตุลาคม พ.ศ. 2566
(Valid from) (30 October B.E.2566 (2023))

ถึงวันที่ 8 กันยายน พ.ศ. 2571
(Until) (8 September B.E.2571 (2028))

สถานภาพห้องปฏิบัติการ
(Laboratory status)

☒ถาวร
(Permanent)

☒นอกสถานที่
(Site)

☐ชั่วคราว
(Temporary)

☐เคลื่อนที่
(Mobile)

☐หลายสถานที่
(Multisite)

สาขาการทดสอบ (Field of Testing)	รายการทดสอบ (Parameter)	วิธีทดสอบ (Test Method)
<p>สาขาสสิ่งแวดล้อม (environmental field)</p> <p>4. บรรยากาศทั่วไป (ต่อ) (ambient air) (cont.)</p>	<p>- สารอินทรีย์ระเหยง่าย (Volatile organic compounds, VOCs)</p> <ul style="list-style-type: none"> อะคริโนไนไทรล์ (Acrylonitrile) 0.04 $\mu\text{g}/\text{m}^3$ ถึง 43.00 $\mu\text{g}/\text{m}^3$ (0.02 ppbv ถึง 20.00 ppbv) ไดคลอโรมีเทน (Dichloromethane) 0.14 $\mu\text{g}/\text{m}^3$ to 69.00 $\mu\text{g}/\text{m}^3$ (0.04 ppbv ถึง 20.00 ppbv) คาร์บอนไดซัลไฟด์ (Carbon disulfide) 0.06 $\mu\text{g}/\text{m}^3$ ถึง 62.00 $\mu\text{g}/\text{m}^3$ (0.02 ppbv ถึง 20.00 ppbv) ไตรคลอโรมีเทน (Trichloromethane) 0.20 $\mu\text{g}/\text{m}^3$ ถึง 97.00 $\mu\text{g}/\text{m}^3$ (0.04 ppbv ถึง 20.00 ppbv) 1,2-ไดคลอโรอีเทน (1,2-dichloroethane) 0.08 $\mu\text{g}/\text{m}^3$ ถึง 80.00 $\mu\text{g}/\text{m}^3$ (0.02 ppbv ถึง 20.00 ppbv) 	<p>- WI-7.2-1-24 based on US EPA , Compendium Method TO-15 , EPA/625/R-96/010b, Second edition, January 1999</p> <p><i>W</i></p>

รายละเอียดสาขาและขอบข่ายใบรับรองห้องปฏิบัติการ
(Scope of Accreditation for Testing)

ใบรับรองเลขที่ 24-LB0026
(Certification No. 24-LB0026)



ฉบับที่ 02
(Issue No.02)

ออกให้ตั้งแต่วันที่ 30 ตุลาคม พ.ศ. 2566
(Valid from) (30 October B.E.2566 (2023))

ถึงวันที่ 8 กันยายน พ.ศ. 2571
(Until) (8 September B.E.2571 (2028))

สถานภาพห้องปฏิบัติการ
(Laboratory status)

☒ถาวร
(Permanent)

☒นอกสถานที่
(Site)

☐ชั่วคราว
(Temporary)

☐เคลื่อนที่
(Mobile)

☐หลายสถานที่
(Multisite)

สาขาการทดสอบ (Field of Testing)	รายการทดสอบ (Parameter)	วิธีทดสอบ (Test Method)
<p>สาขาสสิ่งแวดล้อม (environmental field)</p> <p>4. บรรยากาศทั่วไป (ต่อ) (ambient air) (cont.)</p>	<p>- สารอินทรีย์ระเหยง่าย (Volatile organic compounds ,VOCs)</p> <ul style="list-style-type: none"> • เบนซีน (Benzene) 0.06 $\mu\text{g}/\text{m}^3$ ถึง 63.00 $\mu\text{g}/\text{m}^3$ (0.02 ppbv ถึง 20.00 ppbv) • คาร์บอนเตตระคลอไรด์ (Carbon tetrachloride) 0.25 $\mu\text{g}/\text{m}^3$ ถึง 125 $\mu\text{g}/\text{m}^3$ (0.04 ppbv ถึง 20.00 ppbv) • ไตรคลอโรเอทิลีน (Trichloroethylene) 0.21 $\mu\text{g}/\text{m}^3$ ถึง 107 $\mu\text{g}/\text{m}^3$ (0.04 ppbv ถึง 20.00 ppbv) • 1,2-ไดคลอโรโพรเพน (1,2-dichloropropane) 0.18 $\mu\text{g}/\text{m}^3$ ถึง 92.00 $\mu\text{g}/\text{m}^3$ (0.04 ppbv ถึง 20.00 ppbv) • เตตระคลอโรเอทิลีน (Tetrachloroethylene) 0.27 $\mu\text{g}/\text{m}^3$ ถึง 135 $\mu\text{g}/\text{m}^3$ (0.04 ppbv ถึง 20.00 ppbv) 	<p>- WI-7.2-1-24 based on US EPA , Compendium Method TO-15 , EPA/625/R-96/010b, Second edition, January 1999</p>

รายละเอียดสาขาและขอบข่ายใบรับรองห้องปฏิบัติการ
(Scope of Accreditation for Testing)

ใบรับรองเลขที่ 24-LB0026
(Certification No. 24-LB0026)



ฉบับที่ 02
(Issue No.02)

ออกให้ตั้งแต่วันที่ 30 ตุลาคม พ.ศ. 2566
(Valid from) (30 October B.E.2566 (2023))

ถึงวันที่ 8 กันยายน พ.ศ. 2571
(Until) (8 September B.E.2571 (2028))

สถานภาพห้องปฏิบัติการ
(Laboratory status)

☒ถาวร
(Permanent)

☒นอกสถานที่
(Site)

☐ชั่วคราว
(Temporary)

☐เคลื่อนที่
(Mobile)

☐หลายสถานที่
(Multisite)

สาขาการทดสอบ (Field of Testing)	รายการทดสอบ (Parameter)	วิธีทดสอบ (Test Method)
<p>สาขาสสิ่งแวดล้อม (environmental field)</p> <p>4. บรรยากาศทั่วไป (ต่อ) (ambient air) (cont.)</p>	<p>- สารอินทรีย์ระเหยง่าย (Volatile organic compounds ,VOCs)</p> <ul style="list-style-type: none"> • 1,2-ไดโบรมโอเอเทน (1,2-dibromoethane) 0.31 $\mu\text{g}/\text{m}^3$ ถึง 153 $\mu\text{g}/\text{m}^3$ (0.04 ppbv ถึง 20.00 ppbv) • 1,1,2,2-เตตระคลอโรเอเทน (1,1,2,2-tetrachloroethane) 0.69 $\mu\text{g}/\text{m}^3$ ถึง 137 $\mu\text{g}/\text{m}^3$ (0.10 ppbv ถึง 20.00 ppbv) • เบนซิลคลอไรด์ (Benzyl chloride) 0.52 $\mu\text{g}/\text{m}^3$ ถึง 103 $\mu\text{g}/\text{m}^3$ (0.10 ppbv ถึง 20.00 ppbv) • 1,4-ไดคลอโรเบนซีน (1,4-dichlorobenzene) 0.24 $\mu\text{g}/\text{m}^3$ ถึง 120 $\mu\text{g}/\text{m}^3$ (0.04 ppbv ถึง 20.00 ppbv) 	<p>- WI-7.2-1-24 based on US EPA , Compendium Method TO-15 , EPA/625/R-96/010b, Second edition, January 1999</p>

ภาคผนวก ซ

ใบอนุญาตเป็นนิติบุคคลผู้ให้บริการตรวจวัดและวิเคราะห์
สถานะการทำงานเกี่ยวกับระดับเสียง



แบบ กภ.บุญ
นิติบุคคล

กรมสวัสดิการและคุ้มครองแรงงาน

ใบอนุญาต

เป็นนิติบุคคลผู้ให้บริการตรวจวัดและวิเคราะห์สภาวะการทำงานเกี่ยวกับระดับเสียง

ใบอนุญาตเลขที่ ๐๔๐๓-๐๓-๒๕๖๕-๐๐๔๘

อนุญาตให้.....บริษัท ซีคอน จำกัด.....

เลขทะเบียนนิติบุคคล ๐๑๐๕๕๓๖๐๐๐๗๗๖.....

ตั้งอยู่ เลขที่ ๒๓๙ ถนนริมคลองประปา แขวงบางซื่อ เขตบางซื่อ กรุงเทพมหานคร.....

เป็นนิติบุคคลผู้ให้บริการด้านความปลอดภัย อาชีวอนามัย และสภาพแวดล้อมในการทำงาน ตามกฎกระทรวงกำหนดมาตรฐานในการบริหาร จัดการ และดำเนินการด้านความปลอดภัย อาชีวอนามัย และสภาพแวดล้อมในการทำงานเกี่ยวกับความร้อน แสงสว่าง และเสียง พ.ศ. ๒๕๕๙ ในการตรวจวัดและวิเคราะห์สภาวะการทำงานเกี่ยวกับระดับเสียง ประกอบกับกฎกระทรวงการขึ้นทะเบียนและการอนุญาตให้บริการเพื่อส่งเสริม ความปลอดภัย อาชีวอนามัย และสภาพแวดล้อมในการทำงาน พ.ศ. ๒๕๖๔ แห่งพระราชบัญญัติความปลอดภัย อาชีวอนามัย และสภาพแวดล้อมในการทำงาน พ.ศ. ๒๕๕๔ โดยมีบุคลากร จำนวน ๕ ราย ดังรายชื่อแนบท้ายใบอนุญาตนี้

ทั้งนี้ ตั้งแต่วันที่ ๑๗ มิถุนายน พ.ศ. ๒๕๖๕ ถึงวันที่ ๑๖ มิถุนายน พ.ศ. ๒๕๖๘

ให้ไว้ ณ วันที่ ๑๗ มิถุนายน พ.ศ. ๒๕๖๕

(นายสมพจน์ กวางแก้ว)

รองอธิบดี ปฏิบัติราชการแทน

อธิบดีกรมสวัสดิการและคุ้มครองแรงงาน

เลขทะเบียนควบคุม

ข-๑๑-๐๔๐๓-๐๔๘-๐๑-๖๕

(ลงนาม).....(นายทะเบียน)

(นายศักดิ์ศิลป์ ตูลาธร)

ตำแหน่ง ผู้อำนวยการกองความปลอดภัยแรงงาน

รายชื่อบุคลากรแนบท้ายใบอนุญาต
เป็นนิติบุคคลผู้ให้บริการตรวจวัดและวิเคราะห์สภาวะการทำงานเกี่ยวกับระดับเสียง
ของบริษัท ซีคोट จำกัด

ใบอนุญาตเลขที่ ๐๔๐๓-๐๓-๒๕๖๕-๐๐๔๘

- | | |
|-------------------|---------------|
| ๑. นางสาวสุนันทา | ศิริวัฒนานนท์ |
| ๒. นางสาวกนิษฐา | เจริญเชื้อ |
| ๓. นางสาวปัทมวรรณ | สุวรรณวิโรจน์ |
| ๔. นางสาวอลิษา | คณิธรานนท์ |
| ๕. นางสาวชนิตา | หล้าสาย |

ทั้งนี้ ตั้งแต่วันที่ ๑๗ มิถุนายน พ.ศ. ๒๕๖๕ ถึงวันที่ ๑๖ มิถุนายน พ.ศ. ๒๕๖๘

ให้ไว้ ณ วันที่ ๑๗ มิถุนายน พ.ศ. ๒๕๖๕



(นายสมพจน์ กวางแก้ว)

รองอธิบดี ปฏิบัติราชการแทน
อธิบดีกรมสวัสดิการและคุ้มครองแรงงาน

รายชื่อบุคลากร (เพิ่มเติม)
แนบท้ายใบอนุญาตเป็นนิติบุคคลผู้ให้บริการตรวจวัดและวิเคราะห์สภาวะการทำงานเกี่ยวกับระดับเสียง
ของบริษัท ซีคोट จำกัด

ใบอนุญาตเลขที่ ๐๔๐๓-๐๓-๒๕๖๕-๐๐๔๘

- | | |
|-------------------|-------------|
| ๑. นางสาวศลิษา | อินริย์ |
| ๒. นางสาวมาริยาณี | ยาแวน |
| ๓. นางสาววิระยา | ปัจฉิมบุรณ์ |

ทั้งนี้ ตั้งแต่วันที่ ๑๓ มกราคม พ.ศ. ๒๕๖๖ ถึงวันที่ ๑๖ มิถุนายน พ.ศ. ๒๕๖๘

ให้ไว้ ณ วันที่ ๑๓ มกราคม พ.ศ. ๒๕๖๖



(นายสมพจน์ กวางแก้ว)

รองอธิบดี ปฏิบัติราชการแทน
อธิบดีกรมสวัสดิการและคุ้มครองแรงงาน

รายชื่อบุคลากร (เพิ่มเติม)

แนบท้ายใบอนุญาตเป็นนิติบุคคลผู้ให้บริการตรวจวัดและวิเคราะห์สภาวะการทำงานเกี่ยวกับระดับเสียง

ของบริษัท ซีคोट จำกัด

ใบอนุญาตเลขที่ ๐๔๐๓-๐๓-๒๕๖๕-๐๐๔๘

๑. นายพงศ์ศิริ จักรแก้ว

ทั้งนี้ ตั้งแต่วันที่ ๒๐ มีนาคม พ.ศ. ๒๕๖๘ ถึงวันที่ ๑๖ มิถุนายน พ.ศ. ๒๕๖๘

ให้ไว้ ณ วันที่ ๒๐ มีนาคม พ.ศ. ๒๕๖๘



(นายศักดิ์ศิลป์ ตูลาธร)

ผู้ตรวจราชการกรม ปฏิบัติราชการแทน

อธิบดีกรมสวัสดิการและคุ้มครองแรงงาน

ภาคผนวก ฅ

ใบอนุญาตเป็นนิติบุคคลผู้ให้บริการตรวจวัดระดับความเข้มข้นของ
สารเคมีอันตรายในบรรยากาศของสถานที่ทำงานและสถานที่เก็บรักษา
สารเคมีอันตราย



แบบ กก.บญ
นิติบุคคล

กรมสวัสดิการและคุ้มครองแรงงาน

ใบอนุญาต

เป็นนิติบุคคลผู้ให้บริการตรวจวัดระดับความเข้มข้นของสารเคมีอันตราย
ในบรรยากาศของสถานที่ทำงานและสถานที่เก็บรักษาสารเคมีอันตราย

ใบอนุญาตเลขที่ ๑๒๐๑-๐๓-๒๕๖๕-๐๐๔๙

อนุญาตให้ บริษัท ซีคอน จำกัด

เลขทะเบียนนิติบุคคล ๑๑๐๕๕๓๖๐๐๐๙๗๖

ตั้งอยู่ เลขที่ ๒๓๙ ถนนริมคลองประปา แขวงบางซื่อ เขตบางซื่อ กรุงเทพมหานคร
เป็นนิติบุคคลผู้ให้บริการด้านความปลอดภัย อาชีวอนามัย และสภาพแวดล้อมในการทำงาน ตามกฎกระทรวง
กำหนดมาตรฐานในการบริหาร จัดการ และดำเนินการด้านความปลอดภัย อาชีวอนามัย และสภาพแวดล้อม
ในการทำงานเกี่ยวกับสารเคมีอันตราย พ.ศ. ๒๕๕๖ ในการเป็นผู้ให้บริการตรวจวัดระดับความเข้มข้น
ของสารเคมีอันตรายในบรรยากาศของสถานที่ทำงานและสถานที่เก็บรักษาสารเคมีอันตราย ประกอบกับ
กฎกระทรวงการขึ้นทะเบียนและการอนุญาตให้บริการเพื่อส่งเสริมความปลอดภัย อาชีวอนามัย และสภาพแวดล้อม
ในการทำงาน พ.ศ. ๒๕๖๔ แห่งพระราชบัญญัติความปลอดภัย อาชีวอนามัย และสภาพแวดล้อมในการทำงาน
พ.ศ. ๒๕๕๔ โดยมีบุคลากร จำนวน ๑๔ ราย ดังรายชื่อแนบท้ายใบอนุญาตนี้

ทั้งนี้ ตั้งแต่วันที่ ๑๔ มิถุนายน พ.ศ. ๒๕๖๕ ถึงวันที่ ๑๓ มิถุนายน พ.ศ. ๒๕๖๘

ให้ไว้ ณ วันที่ ๑๔ มิถุนายน พ.ศ. ๒๕๖๕

(นายสมพจน์ กวางแก้ว)

รองอธิบดี ปฏิบัติราชการแทน

อธิบดีกรมสวัสดิการและคุ้มครองแรงงาน

เลขทะเบียนควบคุม

ข-๑๑-๐๒๐๑-๐๔๙-๐๓-๖๕

(ลงนาม)..... (นายทะเบียน)

(นายศักดิ์ศิลป์ ตูลาธร)

ผู้อำนวยการกองความปลอดภัยแรงงาน

รายชื่อบุคลากรแนบท้ายใบอนุญาต
เป็นนิติบุคคลผู้ให้บริการตรวจวัดระดับความเข้มข้นของสารเคมีอันตรายในบรรยากาศของสถานที่ทำงาน
และสถานที่เก็บรักษาสารเคมีอันตราย
ของบริษัท ซีคोट จำกัด
ใบอนุญาตเลขที่ ๐๒๐๑-๐๓-๒๕๖๕-๐๐๔๔

๑. นายชิตพล	สมประสงค์
๒. นายอนิวัฒน์	ทิมวันนา
๓. นายศิวะนนท์	กุลวงษ์
๔. นายวัชรกานต์	ประมาคะเต
๕. นายธนโชติ	ช่างลือ
๖. นายกิตติพงษ์	ทะเกิงสุข
๗. นายจิรวัดน์	โคตรคำหาญ
๘. นายศุภกิจ	ดีมุภา
๙. นางสาวธัญลักษณ์	โยธา
๑๐. นางสาวทิพย์สุดา	วรรณการ
๑๑. นางสาวสายธาร	ภูเขียว
๑๒. นายภาคภูมิ	แทนไทย
๑๓. นายธนาวุฒิ	ด่วนแสง
๑๔. นายรัตนชัย	ชอบทำกิจ

ทั้งนี้ ตั้งแต่วันที่ ๑๕ มิถุนายน พ.ศ. ๒๕๖๕ ถึงวันที่ ๑๓ มิถุนายน พ.ศ. ๒๕๖๘

ให้ไว้ ณ วันที่ ๑๕ มิถุนายน พ.ศ. ๒๕๖๕



(นายสมพจน์ กวางแก้ว)


รองอธิบดี ปฏิบัติราชการแทน
อธิบดีกรมสวัสดิการและคุ้มครองแรงงาน

รายชื่อบุคลากร (เพิ่มเติม)
แนบท้ายใบอนุญาตเป็นนิติบุคคลผู้ให้บริการตรวจวัดระดับความเข้มข้นของสารเคมีอันตราย
ในบรรยากาศของสถานที่ทำงานและสถานที่เก็บรักษาสารเคมีอันตราย
ของบริษัท ซีคोट จำกัด
ใบอนุญาตเลขที่ ๐๒๐๑-๐๓-๒๕๖๕-๐๐๔๔

๑. นางสาวศลิษา	อินริย์
๒. นางสาววิระยา	ปัจฉิมบุรณ์
๓. นายณัฐดนัย	กฤษณะโสม
๔. นายณัฐชัย	ไชยโคตร
๕. นายพงศ์ศิริ	จักรแก้ว
๖. นายอรรถชัย	นวนนัม

ทั้งนี้ ตั้งแต่วันที่ ๓๐ เมษายน พ.ศ. ๒๕๖๘ ถึงวันที่ ๑๓ มิถุนายน พ.ศ. ๒๕๖๘

ให้ไว้ ณ วันที่ ๓๐ เมษายน พ.ศ. ๒๕๖๘



(นายศักดิ์ศิลป์ ตูลาธร)
ผู้ตรวจราชการกรม ปฏิบัติราชการแทน
อธิบดีกรมสวัสดิการและคุ้มครองแรงงาน



แบบ กภ.บุญ
นิติบุคคล

กรมสวัสดิการและคุ้มครองแรงงาน
ใบอนุญาต
เป็นนิติบุคคลผู้ให้บริการตรวจวัดระดับความเข้มข้นของสารเคมีอันตราย
ในบรรยากาศของสถานที่ทำงานและสถานที่เก็บรักษาสารเคมีอันตราย

ใบอนุญาตเลขที่ ๐๒๐๑-๐๓-๒๕๖๕-๐๐๔๙

อนุญาตให้ บริษัท ชีคอต จำกัด

เลขทะเบียนนิติบุคคล ๐๑๑๕๕๗๖๐๐๑๙๗๖

ตั้งอยู่ เลขที่ ๒๓๙ ถนนริมคลองประปา แขวงบางซื่อ เขตบางซื่อ กรุงเทพมหานคร

เป็นนิติบุคคลผู้ให้บริการด้านความปลอดภัย อาชีวอนามัย และสภาพแวดล้อมในการทำงาน ตามกฎกระทรวง
กำหนดมาตรฐานในการบริหาร จัดการ และดำเนินการด้านความปลอดภัย อาชีวอนามัย และสภาพแวดล้อม
ในการทำงานเกี่ยวกับสารเคมีอันตราย พ.ศ. ๒๕๕๖ ในการเป็นผู้ให้บริการตรวจวัดระดับความเข้มข้น
ของสารเคมีอันตรายในบรรยากาศของสถานที่ทำงานและสถานที่เก็บรักษาสารเคมีอันตราย ประกอบกับ
กฎกระทรวงการขึ้นทะเบียนและการอนุญาตให้บริการเพื่อส่งเสริมความปลอดภัย อาชีวอนามัย และสภาพแวดล้อม
ในการทำงาน พ.ศ. ๒๕๖๔ แห่งพระราชบัญญัติความปลอดภัย อาชีวอนามัย และสภาพแวดล้อมในการทำงาน
พ.ศ. ๒๕๕๔ โดยมีบุคลากร จำนวน ๑๕ ราย และรายการเครื่องมือตรวจวัด จำนวน ๕๕ เครื่อง ดังรายละเอียด
แนบท้ายใบอนุญาตนี้

ทั้งนี้ ตั้งแต่วันที่ ๑๔ มิถุนายน พ.ศ. ๒๕๖๘ ถึงวันที่ ๑๓ มิถุนายน พ.ศ. ๒๕๗๑

ให้ไว้ ณ วันที่ ๒๓ พฤษภาคม พ.ศ. ๒๕๖๘

(นายศักดิ์ศิลป์ ตูลาธร)

ผู้ตรวจราชการกรม ปฏิบัติราชการแทน
อธิบดีกรมสวัสดิการและคุ้มครองแรงงาน

เลขทะเบียนควบคุม
ต-๑๑-๐๒๐๑-๐๕๐-๐๒-๖๘

(ลงนาม).....(นายทะเบียน)
(นางสาวสุวดี ทวีสุข)
ผู้อำนวยการกองความปลอดภัยแรงงาน


รายชื่อบุคลากรแนบท้ายใบอนุญาต
เป็นนิติบุคคลผู้ให้บริการตรวจวัดระดับความเข้มข้นของสารเคมีอันตรายในบรรยากาศของสถานที่ทำงาน
และสถานที่เก็บรักษาสารเคมีอันตราย
ของบริษัท ซีคอฟ จำกัด

ใบอนุญาตเลขที่ ๐๒๐๑-๐๓-๒๕๖๕-๐๐๔๙

๑. นายชิตพล	สมประสงค์
๒. นายอนิวัฒน์	พิมพ์นนา
๓. นายศิวนนท์	กุลวงษ์
๔. นายธนโชติ	ช่างหล่อ
๕. นายกิตติพงศ์	ตะเกิงสุข
๖. นายจิรวุฒิ	โคตรคำหาญ
๗. นายศุภกิจ	ตะมุภา
๘. นางสาวทิพย์สุดา	วรรณการ
๙. นายธนาวุฒิ	ด่วนแสง
๑๐. นางสาวศลิษา	อินริย์
๑๑. นางสาววิระยา	ปัจฉิมบุรณ์
๑๒. นายณัฐดนัย	กฤษณะโสม
๑๓. นายณัฐชัย	ไชยโคตร
๑๔. นายพงศ์ศิริ	จักรแก้ว
๑๕. นายอรรถชัย	นวนนิม

ทั้งนี้ ตั้งแต่วันที่ ๑๔ มิถุนายน พ.ศ. ๒๕๖๘ ถึงวันที่ ๑๓ มิถุนายน พ.ศ. ๒๕๗๑

ให้ไว้ ณ วันที่ ๒๓ พฤษภาคม พ.ศ. ๒๕๖๘



(นายศักดิ์ศิลป์ ตูลาธร)

ผู้ตรวจราชการกรม ปฏิบัติราชการแทน
อธิบดีกรมสวัสดิการและคุ้มครองแรงงาน

ภาคผนวก ญ

ใบอนุญาตเป็นนิติบุคคลผู้ให้บริการวิเคราะห์ระดับความเข้มข้นของ
สารเคมีอันตรายในบรรยากาศของสถานที่ทำงานและสถานที่เก็บรักษา
สารเคมีอันตราย



แบบ กบ.บุญ
นิติบุคคล

กรมสวัสดิการและคุ้มครองแรงงาน

ใบอนุญาต

เป็นนิติบุคคลผู้ให้บริการวิเคราะห์ระดับความเข้มข้นของสารเคมีอันตราย
ในบรรยากาศของสถานที่ทำงานและสถานที่เก็บรักษาสารเคมีอันตราย

ใบอนุญาตเลขที่ ๐๒๐๒-๐๓-๒๕๖๕-๐๐๓๔

อนุญาตให้ บริษัท ซีคอน จำกัด

เลขทะเบียนนิติบุคคล ๐๑๐๕๕๓๖๐๐๐๙๗๖

ตั้งอยู่ เลขที่ ๒๓๙ ถนนริมคลองประปา แขวงบางซื่อ เขตบางซื่อ กรุงเทพมหานคร

เป็นนิติบุคคลผู้ให้บริการด้านความปลอดภัย อาชีวอนามัย และสภาพแวดล้อมในการทำงาน ตามกฎกระทรวง
กำหนดมาตรฐานในการบริหาร จัดการ และดำเนินการด้านความปลอดภัย อาชีวอนามัย และสภาพแวดล้อม
ในการทำงานเกี่ยวกับสารเคมีอันตราย พ.ศ. ๒๕๕๖ ในการเป็นผู้ให้บริการวิเคราะห์ระดับความเข้มข้น
ของสารเคมีอันตรายในบรรยากาศของสถานที่ทำงานและสถานที่เก็บรักษาสารเคมีอันตราย ประกอบกับ
กฎกระทรวงการขึ้นทะเบียนและการอนุญาตให้บริการเพื่อส่งเสริมความปลอดภัย อาชีวอนามัย และสภาพแวดล้อม
ในการทำงาน พ.ศ. ๒๕๖๔ แห่งพระราชบัญญัติความปลอดภัย อาชีวอนามัย และสภาพแวดล้อมในการทำงาน
พ.ศ. ๒๕๕๔ โดยมีบุคลากร จำนวน ๑๔ ราย ดังรายชื่อแนบท้ายใบอนุญาตนี้

ทั้งนี้ ตั้งแต่วันที่ ๑๔ มิถุนายน พ.ศ. ๒๕๖๕ ถึงวันที่ ๑๓ มิถุนายน พ.ศ. ๒๕๖๘

ให้ไว้ ณ วันที่ ๑๔ มิถุนายน พ.ศ. ๒๕๖๕

(นายสมพจน์ กวางแก้ว)

รองอธิบดี ปฏิบัติราชการแทน

อธิบดีกรมสวัสดิการและคุ้มครองแรงงาน

เลขทะเบียนควบคุม

ข-๑๑-๐๒๐๒-๐๓๔-๐๑-๖๕

(ลงนาม).....(นายทะเบียน)

(นายศักดิ์ศิลป์ ตูลาธร)

ผู้อำนวยการกองความปลอดภัยแรงงาน

รายชื่อบุคลากรแนบท้ายใบอนุญาต
เป็นนิติบุคคลผู้ให้บริการวิเคราะห์ระดับความเข้มข้นของสารเคมีอันตรายในบรรยากาศของสถานที่ทำงาน
และสถานที่เก็บรักษาสารเคมีอันตราย
ของบริษัท ซีคอท จำกัด
ใบอนุญาตเลขที่ ๐๒๐๒-๐๓-๒๕๖๕-๐๐๓๔

๑. นางสาวนริสา	ภูสรเพ็ชญ์
๒. นางสาวอารยา	ทิพย์รักษ์
๓. นางสาวศิริวรรณ	ฉิมสง่า
๔. นางสาวสุธาทิพย์	เทียนเตี้ย
๕. นางสาวพรนภา	บุตรธรรม
๖. นางสาวธารินี	อาจปลิว
๗. นางสาวกฤษณา	จันทุม
๘. นางสาวพัชรา	สมานฉันท
๙. นางสาวจณิสตา	ก้อยอ่อน
๑๐. นางสาวศศิภา	ใจดี
๑๑. นางสาวจุฑารัตน์	แจ่มเรือน
๑๒. นางสาวณัฐศิริ	เลิศธีรพัฒน์
๑๓. นางสาวสิญญลักษณ์	อินทรประสิทธิ์
๑๔. นางสาวสุตาพร	สุนทร

ทั้งนี้ ตั้งแต่วันที่ ๑๔ มิถุนายน พ.ศ. ๒๕๖๕ ถึงวันที่ ๑๓ มิถุนายน พ.ศ. ๒๕๖๘

ให้ไว้ ณ วันที่ ๑๔ มิถุนายน พ.ศ. ๒๕๖๕



(นายสมพจน์ กวางแก้ว)

รองอธิบดี ปฏิบัติราชการแทน
อธิบดีกรมสวัสดิการและคุ้มครองแรงงาน

รายชื่อบุคลากรแนบท้ายใบอนุญาต (เพิ่มเติม)
เป็นนิติบุคคลผู้ให้บริการวิเคราะห์ระดับความเข้มข้นของสารเคมีอันตรายในบรรยากาศของสถานที่ทำงาน
และสถานที่เก็บรักษาสารเคมีอันตราย
ของบริษัท ซีคอท จำกัด
ใบอนุญาตเลขที่ ๐๒๐๒-๐๓-๒๕๖๕-๐๐๓๔

๑. นางสาวสุรางคณา	มูลพิจิตร
๒. นางสาวกานต์สินี	รุจิระพงศ์ชัย
๓. นางสาวปวีศา	มากักดี

ทั้งนี้ ตั้งแต่วันที่ ๓๐ เมษายน พ.ศ. ๒๕๖๘ ถึงวันที่ ๑๓ มิถุนายน พ.ศ. ๒๕๖๘

ให้ไว้ ณ วันที่ ๓๐ เมษายน พ.ศ. ๒๕๖๘



(นายศักดิ์ศิลป์ ตูลาร)

ผู้ตรวจราชการกรม ปฏิบัติราชการแทน
อธิบดีกรมสวัสดิการและคุ้มครองแรงงาน



แบบ ก.ภ.บุญ
นิติบุคคล

กรมสวัสดิการและคุ้มครองแรงงาน

ใบอนุญาต

เป็นนิติบุคคลผู้ให้บริการวิเคราะห์ระดับความเข้มข้นของสารเคมีอันตราย
ในบรรยากาศของสถานที่ทำงานและสถานที่เก็บรักษาสารเคมีอันตราย

ใบอนุญาตเลขที่ ๐๒๐๒-๐๓-๒๕๖๕-๐๐๓๔

อนุญาตให้ บริษัท ซีคอนท์ จำกัด

เลขทะเบียนนิติบุคคล ๐๑๐๕๕๓๖๐๐๐๙๗๖

ตั้งอยู่ เลขที่ ๒๓๙ ถนนริมคลองประปา แขวงบางซื่อ เขตบางซื่อ กรุงเทพมหานคร

เป็นนิติบุคคลผู้ให้บริการด้านความปลอดภัย อาชีวอนามัย และสภาพแวดล้อมในการทำงาน ตามกฎกระทรวง
กำหนดมาตรฐานในการบริหาร จัดการ และดำเนินการด้านความปลอดภัย อาชีวอนามัย และสภาพแวดล้อม
ในการทำงานเกี่ยวกับสารเคมีอันตราย พ.ศ. ๒๕๕๖ ในการเป็นผู้ให้บริการวิเคราะห์ระดับความเข้มข้น
ของสารเคมีอันตรายในบรรยากาศของสถานที่ทำงานและสถานที่เก็บรักษาสารเคมีอันตราย ประกอบกับ
กฎกระทรวงการขึ้นทะเบียนและการอนุญาตให้บริการเพื่อส่งเสริมความปลอดภัย อาชีวอนามัย และสภาพแวดล้อม
ในการทำงาน พ.ศ. ๒๕๖๔ แห่งพระราชบัญญัติความปลอดภัย อาชีวอนามัย และสภาพแวดล้อมในการทำงาน
พ.ศ. ๒๕๕๔ โดยมีบุคลากร จำนวน ๑๐ ราย และรายการเครื่องมือวิเคราะห์ จำนวน ๙ เครื่อง ดังรายละเอียด
แนบท้ายใบอนุญาตนี้

ทั้งนี้ ตั้งแต่วันที่ ๑๔ มิถุนายน พ.ศ. ๒๕๖๘ ถึงวันที่ ๑๓ มิถุนายน พ.ศ. ๒๕๗๑

ให้ไว้ ณ วันที่ ๒๓ พฤษภาคม พ.ศ. ๒๕๖๘

(นายศักดิ์ศิลป์ ตูลาธร)

ผู้ตรวจราชการกรม ปฏิบัติราชการแทน
อธิบดีกรมสวัสดิการและคุ้มครองแรงงาน

เลขทะเบียนควบคุม

๓-๑๑-๐๒๐๒-๐๓๕-๐๒-๖๘

(ลงนาม)

(นายทะเบียน)

(นางสาวสุวดี ทวีสุข)

ผู้อำนวยการกองความปลอดภัยแรงงาน


รายชื่อบุคลากรแนบท้ายใบอนุญาต
เป็นนิติบุคคลผู้ให้บริการวิเคราะห์ระดับความเข้มข้นของสารเคมีอันตรายในบรรยากาศของสถานที่ทำงาน
และสถานที่เก็บรักษาสารเคมีอันตราย
ของบริษัท ซีคอต จำกัด

ใบอนุญาตเลขที่ ๐๒๐๒-๐๓-๒๕๖๕-๐๐๓๔

- | | |
|--------------------|-------------|
| ๑. นางสาวนริสา | ภูวสรเพ็ชร์ |
| ๒. นางอารยา | ทิพย์รักษ์ |
| ๓. นางสาวศิริวรรณ | นิมสง่า |
| ๔. นางสาวสุธาทิพย์ | เทียนदैย |
| ๕. นางสาวพรนภา | บุตรธรรม |
| ๖. นางสาวธาริณี | อาจปลิว |
| ๗. นางสาวจณิสตา | ก๊วยอ่อน |
| ๘. นางสาวจุฑารัตน์ | แจ่มเรือน |
| ๙. นางสาวสุดาพร | สุนทร |
| ๑๐. นางสาวปวีศา | มากักดี |

ทั้งนี้ ตั้งแต่วันที่ ๑๔ มิถุนายน พ.ศ. ๒๕๖๘ ถึงวันที่ ๑๓ มิถุนายน พ.ศ. ๒๕๗๑

ให้ไว้ ณ วันที่ ๒๗ พฤษภาคม พ.ศ. ๒๕๖๘



(นายศักดิ์ศิลป์ ตูลาธร)

ผู้ตรวจราชการกรม ปฏิบัติราชการแทน
อธิบดีกรมสวัสดิการและคุ้มครองแรงงาน