


ภาคผนวก จ



เอกสารเทียบเครื่องมือที่ใช้ในการตรวจวิเคราะห์

List of Instruments Certification for Air & Noise Quality Analysis

No.	Instrument/Equipment	Parameter	Manufacturer	Model/Serial No.	Calibrator	Certification No.	Date of Calibration	Due date of Calibration	Remark
Ambient									
1	Orifice Transfer Standard Calibrator	Total Suspended Particulate (TSP) Particulate Matter < 10 µm (PM ₁₀)	Thermo Scientific	G25A 1270	Jiranatee Associates Co., Ltd.	CO-004-66	12 Jun 23	11 Jun 25	-
2	U-Tube Manometer	Total Suspended Particulate (TSP) Particulate Matter < 10 µm (PM ₁₀)	Dwyer	1221-36-W/M -	Technology Promotion Association (Thailand-Japan)	24P1252	11 Apr 24	10 Apr 25	-
3	Aneroid Barometer	Total Suspended Particulate (TSP) Particulate Matter < 10 µm (PM ₁₀)	Barigo, Germany	-	Technology Promotion Association (Thailand-Japan)	24P1369	22 Apr 24	21 Apr 25	-
4	Dial Thermo-Hygrometer	Total Suspended Particulate (TSP) Particulate Matter < 10 µm (PM ₁₀)	Barigo, Germany	-	Technology Promotion Association (Thailand-Japan)	24H757	10 Apr 24	9 Apr 25	-
5	Nitrogen Dioxide Analyzer	Nitrogen Dioxide	Thermo Fisher Scientific	42C 0517512000	UAE Consultant Co.,Ltd.	04102024	4 Oct 24	3 Oct 25	-
6	Nitrogen Dioxide Analyzer	Nitrogen Dioxide	Thermo Electron	42C 0517512001	UAE Consultant Co.,Ltd.	11102024	11 Oct 24	10 Oct 25	-
7	Nitrogen Dioxide Analyzer	Nitrogen Dioxide	Thermo Scientific	42i CM08130002	UAE Consultant Co.,Ltd.	17092024	17 Sep 24	16 Sep 25	-
8	Standard Gases (Mixture)	Nitrogen Dioxide	Airgas	EB0162121 2016PSIG	Airgas an Air Liquide company	E05NI91E15A0014	6 Jun 23	6 Jun 31	-
9	Sulphur Dioxide Analyzer	Sulphur Dioxide	Thermo Scientific	43i CM22387065	UAE Consultant Co.,Ltd.	06092024	6 Sep 24	5 Sep 25	-
10	Sulphur Dioxide Analyzer	Sulphur Dioxide	Thermo Scientific	43i CM22387066	UAE Consultant Co.,Ltd.	06092024	6 Sep 24	5 Sep 25	-
11	Sulphur Dioxide Analyzer	Sulphur Dioxide	Thermo Scientific	43i CM22387067	UAE Consultant Co.,Ltd.	15052024	15 May 24	14 May 25	-
12	Standard Gases (Mixture)	Sulphur Dioxide	Airgas	EB0162121 2016PSIG	Airgas an Air Liquide company	E05NI91E15A0014	6 Jun 23	6 Jun 31	-
13	Wind Speed/Wind Direction	WS/WD	Scarlet Tech Ltd.	WL-21 2205DR0114	Thai Meteorological Department	099/24	22 Feb 24	21 Feb 25	-

List of Instruments Certification for Air & Noise Quality Analysis

No.	Instrument/Equipment	Parameter	Manufacturer	Model/Serial No.	Calibrator	Certification No.	Date of Calibration	Due date of Calibration	Remark
Ambient									
14	Sound Level Calibrator (Acoustic Calibrator)	Calibrate Sound Level Meter	Svantek	SV36 107224	Innovative Instrument Co.,Ltd.	24-ACT-091	26 Jun 24	25 Jun 25	-
15	Sound Level Meter	$L_{Aeq} 1\text{ hr}$, $L_{Aeq} 24\text{ hrs}$, L_{Amax} , L_{A90} , L_{Adn}	Larson Davis	LxT1 0007305	Electrical And Electronics Institute Foundation For Industrial Development	CP20240323EA	22 Aug 24	21 Aug 25	-
16	Sound Level Meter	$L_{Aeq} 1\text{ hr}$, $L_{Aeq} 24\text{ hrs}$, L_{Amax} , L_{A90} , L_{Adn}	Larson Davis	LxT1 0007306	Electrical And Electronics Institute Foundation For Industrial Development	CP20240290EA	5 Aug 24	4 Aug 25	-
17	Sound Level Meter	$L_{Aeq} 1\text{ hr}$, $L_{Aeq} 24\text{ hrs}$, L_{Amax} , L_{A90} , L_{Adn}	Larson Davis	LxT1 0007308	Electrical And Electronics Institute Foundation For Industrial Development	CP20240322EA	22 Aug 24	21 Aug 25	-
18	Sound Level Meter	$L_{Aeq} 1\text{ hr}$, $L_{Aeq} 24\text{ hrs}$, L_{Amax} , L_{A90} , L_{Adn}	Larson Davis	LxT1 0007309	Electrical And Electronics Institute Foundation For Industrial Development	CP202340287EA	2 Aug 24	1 Aug 25	-
19	Sound Level Meter	$L_{Aeq} 1\text{ hr}$, $L_{Aeq} 24\text{ hrs}$, L_{Amax} , L_{A90} , L_{Adn}	Larson Davis	LxT1 0007310	Electrical And Electronics Institute Foundation For Industrial Development	CP20240289EA	5 Aug 24	4 Aug 25	-
20	Sound Level Meter	$L_{Aeq} 1\text{ hr}$, $L_{Aeq} 24\text{ hrs}$, L_{Amax} , L_{A90} , L_{Adn}	Larson Davis	LxT1 0007312	Electrical And Electronics Institute Foundation For Industrial Development	CP20240288EA	5 Aug 24	4 Aug 25	-

List of Instruments Certification for Water Quality Analysis

No.	Instrument/Equipment	Parameter	Manufacturer	Model/Serial No.	Calibrator	Certification No.	Date of Calibration	Due date of Calibration	Remark
Water									
1	pH Meter	pH	Ecosence	pH100A JC04740	Technology Promotion Association (Thailand-Japan)	24CH311	13 Mar 24	12 Mar 25	-
2	DO Meter	DO	Horiba	LAQUA-DO210 HE2L0031	Technology Promotion Association (Thailand-Japan)	24TW56	13 Mar 24	12 Mar 25	-
3	Conductivity Meter	Conductivity	Horiba	LAQUA-EC210 HC9L0015	Technology Promotion Association (Thailand-Japan)	24CH322	14 Mar 24	13 Mar 25	-

List of Instruments Certification for Air & Noise Quality Analysis

No.	Instrument/Equipment	Parameter	Manufacturer	Model/Serial No.	Calibrator	Certification No.	Date of Calibration	Due date of Calibration	Remark
Workplace									
1	Primary Flow Calibrator	Calibrate personal pump	TSL Inc	4146 41462317033	Innovative Instrument Co., Ltd.	24-AFM-101	24 May 24	23 May 25	-
2	Aneroid Barometer	Total Dust Respirable Dust	Barigo, Germany	-	Technology Promotion Association (Thailand-Japan)	24P1145	9 Apr 24	8 Apr 25	-
3	Digital Thermo - Hygrometer	Total Dust Respirable Dust	Digicon	TH-02 395034173	Technology Promotion Association (Thailand-Japan)	24H716	10 Apr 24	9 Apr 25	-
4	Thermal Environment Monitor	Heat Meter	3M	QuesTemp 32 TPQ020024	Innovative Instrument Co.,Ltd.	24-TPM-148	21 Mar 24	20 Mar 25	-
5	Thermal Environment Monitor	Heat Meter	3M	QuesTemp 32 TPQ020025	Innovative Instrument Co.,Ltd.	24-TPM-152	21 Apr 24	20 Apr 25	-
6	Sound Level Calibrator (Acoustic Calibrator)	Calibrate Sound Level Meter	Larson Davis	CAL150 6306	Innovative Instrument Co.,Ltd.	24-ACT-067	17 May 24	16 May 25	-
7	Sound Level Meter	L_{Aeq} 8 hours ² L_{Amax}	Rion, Japan	NL-42 00409023	Sithiporn Associates Co., Ltd.	ACL24160	4 Jun 24	3 Jun 25	-
8	Sound Level Meter	L_{Aeq} 8 hours ² L_{Amax}	Rion, Japan	NL-42 00409177	Sithiporn Associates Co., Ltd.	ACL24161	4 Jun 24	3 Jun 25	-

CERTIFICATE OF CALIBRATION

Certificate No. : CO-004-66

Page 1 of 2 Pages

MEASUREMENT ITEM : Top Load Orifice
MANUFACTURER : Anderson Instruments
MODEL/TYPE : G25A
SERIAL NUMBER : 1270
ID NUMBER : UAE.ANV.009/2542
CONDITION AS-RECEIVED : Used item
CUSTOMER : United Analyst and Engineering Consultant Co., Ltd.
81 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong,
Bangkok 10260

RECEIVED DATE : 02 Jun 2023
MEASUREMENT DATE : 02 Jun 2023
ISSUE DATE : 12 Jun 2023

ENVIRONMENTAL CONDITIONS:

Analysis conditions in the laboratory are as follows:

Temperature : 23.0 ± 3.0 °C
Relative Humidity : 55.0 ± 15.0 %RH
Atmospheric Pressure : 1010 ± 10 hPa

CALIBRATION CONDITION:

Preconditioning : 24 hours at ambient conditions.
Measurement Condition : The average values during measurement are 23.3 °C and 55.0%RH.

NOTE: The certificate is valid only to the item calibrated on date and place of calibration.

TABULATION OF RESULTS:

The table on next page give the measured values.

Calibration procedure:
The Orifice gas flow device was calibrated against Standard Rotary Displacement Meter (Roots Meter) Model G65/1MC/V2-0a. The W-CE-004 was used as a calibration guideline.

Traceability:
This certificate provides a traceability of the measurement to recognized the national standards and to realization of the international system of units (SI) through the VSL (National Metrology Institute of Netherlands) via Certificate number: G2221901

Uncertainty of Measurement:
The reported uncertainty of measurement is based on the standard uncertainty multiplied by a coverage factor k=2. Which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty has been determined in accordance with the GUM "Evaluation of measurement data - Guide to the expression of uncertainty in measurement"

MEASUREMENT RESULTS:

The Orifice gas flow device was calibrated by direct comparison method with the Standard Rotary Displacement Meter (Roots Meter). The humid air was used as a medium in the system. The standard conditions are 25 °C (298.15 K) and 760 mmHg for standard temperature and standard pressure respectively.

Table 1: The results of Q Standard calibration data

Plate	Flow rate m ³ /min	Pressure [Pa] mmHg	Temperature [Ta] °C	Temperature [Tm] °C	Ap_meter mmHg	Ap_Orifice inH ₂ O	F	Standard Flow [Qs] m ³ /min
1	0.705	755.787	24.37	23.48	47.401	1.708	1.305	0.661
2	0.999	755.849	23.95	23.54	51.522	3.383	1.333	0.930
3	1.119	755.810	23.39	22.98	35.502	4.448	1.323	1.068
4	1.170	755.752	23.42	23.02	26.462	4.999	1.401	1.131
5	1.425	755.681	23.52	23.12	26.582	7.431	1.708	1.377

Slope (m) : 1.98581
Intercept (b) : -0.00878
Correlation coefficient (r) : 0.99984
Uncertainty (k=2) : 0.015 m³/min

Table 2: The results of Q actual calibration data

Plate	Flow rate m ³ /min	Pressure [Pa] mmHg	Temperature [Ta] °C	Temperature [Tm] °C	Ap_meter mmHg	Ap_Orifice inH ₂ O	F	Standard Flow [Qs] m ³ /min
1	0.705	755.787	24.17	23.48	47.401	1.708	0.820	0.663
2	0.999	755.849	23.95	23.54	51.522	3.383	1.333	0.932
3	1.119	755.810	23.39	22.98	35.502	4.448	1.323	1.068
4	1.170	755.752	23.42	23.02	26.462	4.999	1.401	1.131
5	1.425	755.681	23.52	23.12	26.582	7.431	1.708	1.377

Slope (m) : 1.24382
Intercept (b) : -0.00554
Correlation coefficient (r) : 0.99984
Uncertainty (k=2) : 0.015 m³/min

End of Certificate of Calibration

Calibrated by:
☐ Mr. Serawit Thachulad
☒ Miss Jitraporn Lertsomphol



Approved signatory: _____
Mr. Patinya Booncharoen
Calibration Department Manager



เอกสารไม่ควบคุม

THIS CERTIFICATE REPORT MAY NOT BE REPRODUCED EXCEPT IN FULL UNLESS PERMISSION FOR REPRODUCTION HAS BEEN OBTAINED IN WRITING FROM THE LABORATORY

เอกสารไม่ควบคุม



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
53/44 PATTANAKARN ROAD SOI 18, SUANLIANG, SUANLIANG, BANGKOK 10250
TEL. 0-2717-3000-24 FAX. 0-2719-9484

Certificate of Calibration

Certificate No. : 24P1252
Page : 1 of 2

Equipment : U Tube Manometer
Manufacturer : Dwyer
Model : 1221-36-W/M
Serial No. : -
ID No. : UAE.EFM.078/2566

Condition As-Received: Used Item

Received Date: 03 April 2024

Calibration Date: 11 April 2024

Reference: 2404-0118WSC

Ambient Temperature: (23 ± 2) °C

Relative Humidity: (50 ± 15) %

Atmospheric Pressure: 1011 mbar

Submitted by: United Analyst and Engineering Consultant Co., Ltd.

81 Soi Udomsuk 41, Sukhumvit Road, Bangchak,
Phrakhanong, Bangkok 10260

Procedure used: The calibration was conducted by direct comparison method against Pressure Measuring Instruments Standard according to calibration procedure CP-P04, using * DKD-R 6-1; Calibration of Pressure Gauges * as a guidelines.

Condition of this result of calibration

1. Reference standards instruments :

Instrument	Model	Serial No.	Certificate No.	Due Date
1) Pressure Calibrator	PC106P	1189	MP-0176-23	12 Sep 2024

2. This result of calibration was made on requested at the point specified by customer.

3. Scale and conversion factor is 1 kPa = 4.0146293 inH₂O

4. This instrument was used clean air as pressure media.

5. This instrument was calibrated by applied pressure to high-port (+) side and low-port (-) side open to atmospheric pressure.

6. This instrument was installed in vertical orientation and top of the pressure port was used as the reference level.

7. The certificate is valid only to the item calibrated on date and place of calibration.

8. This Certification is traceable to the International System of Unit maintained through:-

-National Institute of Metrology (Thailand), NSC-ONSC Accredited No. Calibration 0144

Calibrated by : Suksan Khankaw
Issue Date : 17 April 2024

Approved Signatory :

[] Phalinee Prabpaipal
[] Sura Suwannasri
[x] Attapol Panurach

เอกสารไม่ควบคุม



Cart.No.: 24P1252
Page: 2 of 2

Result of calibration:- Without adjustment
Function:- Pressure Measurement
Increasing Pressure

Range: 0 inH₂O to 36 inH₂O
Scale Interval: 0.1 inH₂O (The Second Estimate)

Applied Pressure	High-port side	Low-port side	UUC Indication ΔP	Error
0.00	0.00	0.00	2.00	0.00
2.00	1.00	-1.00	4.00	0.00
4.00	2.00	-2.00	6.00	0.00
6.00	3.00	-3.00	8.00	0.00
8.00	4.00	-4.00	10.00	0.00
10.00	5.00	-5.00	12.00	0.00
12.00	6.00	-6.00	14.05	0.05
14.00	7.00	-7.05	16.05	0.05
16.00	8.00	-8.05	18.05	0.05
18.00	9.00	-9.05	20.10	0.10
20.00	10.00	-10.10	22.10	0.10
22.00	11.00	-11.10	24.10	0.10
24.00	12.00	-12.10	26.10	0.10
26.00	13.00	-13.10	28.10	0.10
28.00	14.00	-14.10	30.10	0.10
30.00	15.00	-15.10	32.10	0.10
32.00	16.00	-16.10	34.15	0.15
34.00	17.05	-17.10	36.00	0.20
35.80	18.00	-18.00		

The uncertainty of measurement was ± 0.11 inH₂O

* ΔP = High-port side - Low-port side

* UUC = Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k=2, providing a level of confidence of approximately 95 %.

-00-

เอกสารไม่ควบคุม



Certificate of Calibration

Certificate No. : 24P1369
Page : 1 of 2

Equipment : Aneroid Barometer
Manufacturer: Barigo
Model :
Serial No. :
ID No. : UAE.ANV.013/2547

This certificate may not be reproduced other than in full,
except with the prior written approval of the head of
Corporate Services 3: Equipment Calibration and Testing Services.

Condition As-Received: Used Item
Received Date: 05 April 2024
Calibration Date: 22 April 2024

Reference: 2404-0243WSC
Ambient Temperature: (23 ± 2) °C
Relative Humidity: (50 ± 15) %
Atmospheric Pressure: 1007 mbar
Submitted by: United Analyst and Engineering Consultant Co.,Ltd.
81 Soi Udomsuk 41, Sukhumvit Road, Bangchak,
Phrakhanong, Bangkok 10260

Procedure used: The calibration was conducted by direct comparison method against Pressure Measuring Instruments
Standard according to calibration procedure CP-P10, using " DKD-R 6-1 ; Calibration of Pressure Gauges " as
a guidelines.

Condition of this result of calibration

1.Reference standards instruments :

Instrument	Model	Serial No.	Certificate No.	Due Date
1) Standard Barometer	DPI142	1422505046	MP-0094-23	03 May 2024

2.This instrument was installed in vertical orientation and center of the dial was used as the reference level.

3.This result of calibration was made on requested at the point specified by customer.

4.Scale and conversion factor is 1 kPa = 7.50062 mmHg

5.This result of calibration instrument was in absolute pressure.

6.This instrument was used clean air as pressure media.

7.The certificate is valid only to the item calibrated on date and place of calibration.

8.This Certification is traceable to the International System of Unit maintained through:-

-National Institute of Metrology Thailand (NIMT)

Calibrated by : Suksan Khankaew
Issue Date : 23 April 2024

Approved Signatory :
[] Phalinee Prabpaipal
[] Sura Suwannasri
[✓] Attapol Panurach

เอกสารไม่ควบคุม



Cert.No.: 24P1369
Page: 2 of 2

Result of calibration:- Without adjustment

Function:- Absolute Pressure Measurement

Range : 720 mmHg to 780 mmHg

Scale Interval : 1 mmHg (The Fifth Estimate)

Increasing Pressure

Applied Pressure (mmHg)	718.40	729.71	740.61	751.07	761.97	773.05	786.91
UUC* Indication (mmHg)	720.0	730.0	740.0	750.0	760.0	770.0	780.0
Error (mmHg)	1.60	0.29	-0.61	-1.07	-1.97	-3.05	-6.91

Decreasing Pressure

Applied Pressure (mmHg)	786.91	772.99	761.71	750.69	740.13	729.35	718.44
UUC* Indication (mmHg)	780.0	770.0	760.0	750.0	740.0	730.0	720.0
Error (mmHg)	-6.91	-2.99	-1.71	-0.69	-0.13	0.65	1.56

The uncertainty of measurement was ± 0.24 mmHg

* UUC = Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied
by a coverage factor $k = 2$, providing a level of confidence of approximately 95 %.

-00-

เอกสารไม่ควบคุม



Certificate of Calibration

Certificate No. : 24H757
Page : 1 of 2

Equipment : Dial Thermo-Hygrometer
Manufacturer: Barigo
Model :
Serial No. :
ID No. : UAE.ANV.132/2550

This certificate may not be reproduced other than in full,
except with the prior written approval of the head of
Corporate Services 3: Equipment Calibration and Testing Services.

Condition As-Received: Used Item
Received Date: 05 April 2024
Calibration Date: 10 April 2024
to 18 April 2024

Reference: 2404-0247WSC
Ambient Temperature: (25 ± 3) °C
Relative Humidity: (50 ± 20) %
Submitted by: United Analyst and Engineering Consultant Co.,Ltd.
81 Soi Udomsuk 41, Sukhumvit Road,
Bangchak, Phrakhanong, Bangkok 10260

Procedure used: Calibration were conducted using in-house calibration procedure CP-H02 according to comparison
with standard chilled mirror sensor for humidity measurement function and comparison with standard
temperature probe for temperature measurement function into humidity / temperature chamber.

Condition of this result of calibration

1.Reference standards instruments :

Instrument	Model	Serial No.	Certificate No.	Due Date
1) Chilled Mirror Hygrometer	Dew Master	44730	21656	02 Aug 2024
2) Handheld Thermometer With Sensor	1521	A5A339	231238	16 Oct 2024

2.The certificate is valid only to the item calibrated on date and place of calibration.

3.This Certification is traceable to the International System of Unit maintained through:-

-Thunder Scientific Corporation, NVLAB Accreditation No. Calibration 200582-0

-Technology Promotion Association (Thailand-Japan), NSC-ONSC Accredited No. Calibration 0006

Calibrated by : Chakrit Waewwanjua
Issue Date : 18 April 2024

Approved Signatory :
[✓] Chakrit Waewwanjua
[] Viporn Tantiyawutti
[] Unnoppol Harachai

เอกสารไม่ควบคุม



Cert. No.: 24H757
Page.: 2 of 2

Result of Calibration:- Without Adjustment

Function: Humidity Measurement.

Reference Temperature	Standard Humidity	UUC* Reading	Error	Uncertainty of Measurement
(°C)	(%R.H.)	(%R.H.)	(%R.H.)	(±%R.H.)
25.0	40.1	41	0.9	1.6
25.0	60.0	61	1.0	1.7
25.0	80.0	76	-4.0	1.8

Result of Calibration:- Without Adjustment

Function: Temperature Measurement.

Standard Temperature	UUC* Reading	Error	Uncertainty of Measurement
(°C)	(°C)	(°C)	(±°C)
20.007	20.5	0.493	0.72
25.032	25.5	0.468	0.72
29.997	30.0	0.003	0.72
35.010	35.0	-0.010	0.72
40.019	39.5	-0.519	0.72

UUC* : Unit Under Calibration

The reported uncertainty of measurement was base on standard uncertainty multiplied
by coverage factor $k = 2.00$, providing confidence level approximately 95%.

-00-

เอกสารไม่ควบคุม

MULTI-POINT GAS TEST REPORT

Test Date : Oct 4, 2024

Equipment : Gas Analyzer (NO₂) Model : 42C
Manufacturer : Thermo Electron Corporation Serial Number : 0517512000


Standard Gas Concentration

Sulphur Dioxide (SO ₂)	42.89	PPM	Manufacturer :	Thermo Scientific
Nitric Oxide (NO)	46.77	PPM	Model :	146i
Methane (CH ₄)	-	PPM	Serial Number :	1180540071
Carbon Monoxide (CO)	965.9			
Cylinder No. :	EB0159156			
Expiration Date :	Nov 6, 2026			

Dilutor Detail

Multi-point gas test data

Reference Value (ppb)	Analyzer Display (ppb)	Difference Error	Percent Error	[% Error]
Level 1 Zero	0.0	0.00	0.00	0.00
Level 2 20.00%	100.0	100.7	0.70	0.70
Level 3 40.00%	200.0	200.5	0.50	0.25
Level 4 60.00%	300.0	300.9	0.90	0.30
Level 5 80.00%	400.0	400.0	0.00	0.00
Remark : Measuring Range 500.0 ppb		Average Difference (%)		
:Acceptable Limit \pm 5%		0.25		

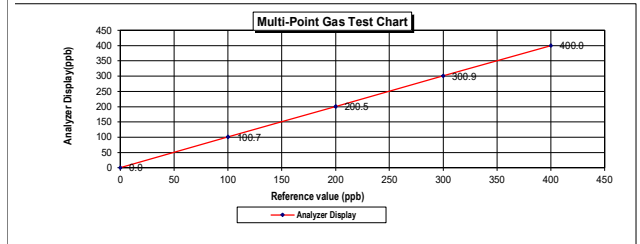

Calculate by *Girishan S*
4 10 2567

Approve by *Prakham K*
4 Oct 2024

MULTI-POINT GAS TEST REPORT

Test Date : Oct 11, 2024

Equipment : Gas Analyzer (NO₂) Model : 42C
Manufacturer : Thermo Electron Corporation Serial Number : 0517512001


Standard Gas Concentration

Sulphur Dioxide (SO ₂)	42.89	PPM	Manufacturer :	Thermo Scientific
Nitric Oxide (NO)	46.77	PPM	Model :	146i
Methane (CH ₄)	-	PPM	Serial Number :	1180540071
Carbon Monoxide (CO)	965.9			
Cylinder No. :	EB0159156			
Expiration Date :	Nov 6, 2026			

Dilutor Detail

Multi-point gas test data

Reference Value (ppb)	Analyzer Display (ppb)	Difference Error	Percent Error	[% Error]
Level 1 Zero	0.0	0.00	0.00	0.00
Level 2 20.00%	100.0	101.7	1.70	1.67
Level 3 40.00%	200.0	200.7	0.70	0.35
Level 4 60.00%	300.0	300.8	0.80	0.27
Level 5 80.00%	400.0	400.0	0.00	0.00
Remark : Measuring Range 500.0 ppb		Average Difference (%)		
:Acceptable Limit \pm 5%		0.46		

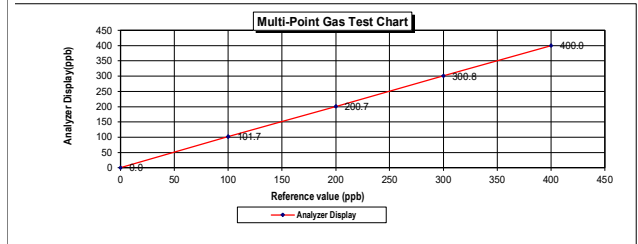

Calculate by *Girishan S*
11 10 2567

Approve by *Prakham K*
11 Oct 2024

MULTI-POINT GAS TEST REPORT

Test Date : Sep 17, 2024

Equipment : Gas Analyzer (NO₂) Model : 42i
Manufacturer : Thermo Scientific Serial Number : CM08130002


Standard Gas Concentration

Sulphur Dioxide (SO ₂)	42.89	PPM	Manufacturer :	Thermo Scientific
Nitric Oxide (NO)	46.77	PPM	Model :	146i
Methane (CH ₄)	-	PPM	Serial Number :	1180540071
Carbon Monoxide (CO)	965.9			
Cylinder No. :	EB0159156			
Expiration Date :	Nov 6, 2026			

Dilutor Detail

Multi-point gas test data

Reference Value (ppb)	Analyzer Display (ppb)	Difference Error	Percent Error	[% Error]
Level 1 Zero	0.0	0.50	0.50	0.50
Level 2 20.00%	100.0	101.6	1.60	1.57
Level 3 40.00%	200.0	200.5	0.50	0.25
Level 4 60.00%	300.0	300.8	0.80	0.27
Level 5 80.00%	400.0	400.0	0.00	0.00
Remark : Measuring Range 500.0 ppb		Average Difference (%)		
:Acceptable Limit \pm 5%		0.52		

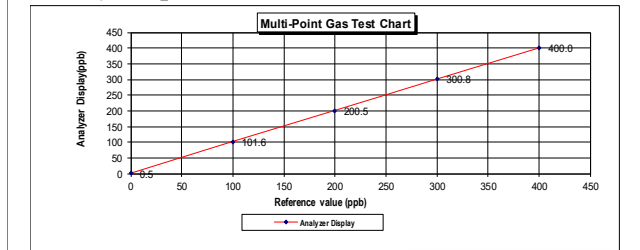

Calculate by *Girishan S*
17 9 2567

Approve by *Prakham K*
17 Sep 2024

CERTIFICATE OF ANALYSIS

Grade of Product: EPA PROTOCOL STANDARD

Customer: AIR LIQUIDE (THAILAND)
LTD--
Part Number: E05N91E15A0014
Cylinder Number: EB0182121
Laboratory: 124 - Plumsteadville - PA
PGVP Number: A12023
Gas Code: CO, CO₂, NO, NO₂, SO₂, BALN
Reference Number: 160-402772205-1
Cylinder Volume: 144.0 CF
Cylinder Pressure: 2015 PSIG
Valve Outlet: 660
Certification Date: Jul 06, 2023
Expiration Date: Jul 06, 2031

Certification performed in accordance with "EPA Traceability Protocol for Assay and Certification of Gaseous Calibration Standards (May 2012)" document EPA-820/R-12-051, using the assay procedures listed. Assay methodology does not require correction for analysis interference. This cylinder has a total analytical uncertainty as stated below with a confidence level of 95%. There are no significant impurities which affect the use of this calibration mixture. All concentrations are on a mole/mole basis unless otherwise noted. The results herein only to the items listed. The report shall not be reproduced except in full without approval of the laboratory. Do Not Use This Cylinder below 100 psig, i.e. 7.7 megapascals.

ANALYTICAL RESULTS				
Component	Requested Concentration	Actual Concentration	Protocol Method	Total Relative Uncertainty
NOX	100.0 PPM	100.4 PPM	G1	\pm 0.9% NIST Traceable
NITRIC OXIDE	100.0 PPM	100.2 PPM	G1	\pm 0.9% NIST Traceable
SULFUR DIOXIDE	100.0 PPM	100.5 PPM	G1	\pm 1.4% NIST Traceable
CARBON MONOXIDE	200.0 PPM	199.2 PPM	G1	\pm 0.3% NIST Traceable
CARBON DIOXIDE	8,000 %	7,982 %	G1	\pm 1.3% NIST Traceable
NITROGEN	Balance			

CALIBRATION STANDARDS				
Type	Lot ID	Cylinder No	Concentration	Uncertainty
GMIS	104202308	CC754364	98.36 PPM NITRIC OXIDE/NITROGEN	\pm 0.4%
PRM	C2219101	AP1514048	100.16 PPM NITRIC OXIDE/NITROGEN	\pm 0.3%
GMIS	2023042525	CC754361	98.62 PPM NITRIC OXIDE/NITROGEN	\pm 0.4%
PRM	12459	D813880	15.01 PPM NITROGEN DIOXIDE/AIR	\pm 1.5%
GMIS	15340202692	EB0130037	9.993 PPM NITROGEN DIOXIDE/NITROGEN	\pm 1.0%
NTRM	160102-22	KAL203626	97.69 PPM SULFUR DIOXIDE/NITROGEN	\pm 0.9%
CO	230801	CC745902	249.47 PPM CARBON MONOXIDE/NITROGEN	\pm 0.3%
NTRM	130606-02	CC411730	13.359 % CARBON DIOXIDE/NITROGEN	\pm 0.5%

ANALYTICAL EQUIPMENT		
Instrument/Make/Model	Analytical Principle	Last Multipoint Calibration
Nicolet iS65 FTIR AUP2010245 CO2	FTIR	Jun 15, 2023
SIEMENS ULTRAMATE6E N1-CR-180	NDIR	Jun 14, 2023
Nicolet iS55 FTIR AUP2010245 NO	FTIR	Jun 29, 2023
Nicolet iS55 FTIR AUP2010245 NO2	FTIR	Jun 15, 2023
Nicolet iS55 FTIR AUP2010245 SO2	FTIR	Jun 08, 2023

Approved for Release

MULTI-POINT GAS TEST REPORT

Test Date : Sep 6, 2026


Equipment : Gas Analyzer (SO₂) Model : 43i
Manufacturer : Thermo SCIENTIFIC Serial Number : CM22387065

Standard Gas Concentration

Sulphur Dioxide (SO ₂)	42.89	PPM	Manufacturer :	Thermo SCIENTIFIC
Nitric Oxide (NO)	46.77	PPM	Model :	146i
Methane (CH ₄)	-	PPM	Serial Number :	1180540071
Carbon Monoxide (CO)	965.9			
Cylinder No. :	EB01159156			
Expiration Date :	Nov 06, 2026			

Multi-point gas test data

Reference Value (ppb)	Analyzer Display (ppb)	Difference Error	Percent Error	[% Error]
Level 1 Zero	0.0	0.00	0.00	0.00
Level 2 20.00%	100.0	100.6	0.60	0.60
Level 3 40.00%	200.0	200.6	0.30	0.30
Level 4 60.00%	300.0	300.9	0.30	0.30
Level 5 80.00%	400.0	400.0	0.00	0.00
Remark : Measuring Range	500.0 ppb	Average Difference (%)		0.24
:Acceptable Limit \pm 5%				

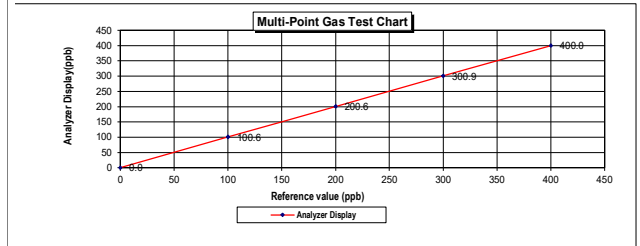

Calculate by *Smthan Cj*
6 / 9 / 2567

Approve by *Phrakhanong*
6 / Sep / 2024

MULTI-POINT GAS TEST REPORT

Test Date : Sep 6, 2024


Equipment : Gas Analyzer (SO₂) Model : 43i
Manufacturer : Thermo SCIENTIFIC Serial Number : CM22387066

Standard Gas Concentration

Sulphur Dioxide (SO ₂)	42.89	PPM	Manufacturer :	Thermo SCIENTIFIC
Nitric Oxide (NO)	46.77	PPM	Model :	146i
Methane (CH ₄)	-	PPM	Serial Number :	1180540071
Carbon Monoxide (CO)	965.9			
Cylinder No. :	EB01159156			
Expiration Date :	Nov 06, 2026			

Multi-point gas test data

Reference Value (ppb)	Analyzer Display (ppb)	Difference Error	Percent Error	[% Error]
Level 1 Zero	0.0	0.00	0.00	0.00
Level 2 20.00%	100.0	100.9	0.90	0.89
Level 3 40.00%	200.0	200.7	0.35	0.35
Level 4 60.00%	300.0	300.7	0.23	0.23
Level 5 80.00%	400.0	400.0	0.00	0.00
Remark : Measuring Range	500.0 ppb	Average Difference (%)		0.29
:Acceptable Limit \pm 5%				

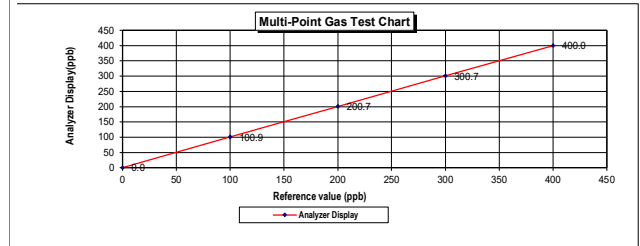

Calculate by *Smthan Cj*
6 / 9 / 2567

Approve by *Phrakhanong*
6 / Sep / 2024

MULTI-POINT GAS TEST REPORT

Test Date : May 15, 2024


Equipment : Gas Analyzer (SO₂) Model : 43i
Manufacturer : Thermo SCIENTIFIC Serial Number : CM22387067

Standard Gas Concentration

Sulphur Dioxide (SO ₂)	44.68	PPM	Manufacturer :	Thermo SCIENTIFIC
Nitric Oxide (NO)	45.94	PPM	Model :	146i
Methane (CH ₄)	-	PPM	Serial Number :	1180540071
Carbon Monoxide (CO)	984.8			
Cylinder No. :	EB0143262			
Expiration Date :	Jun 24, 2024			

Multi-point gas test data

Reference Value (ppb)	Analyzer Display (ppb)	Difference Error	Percent Error	[% Error]
Level 1 Zero	0.0	0.90	0.90	0.90
Level 2 20.00%	100.0	100.8	0.80	0.79
Level 3 40.00%	200.0	200.9	0.45	0.45
Level 4 60.00%	300.0	300.9	0.30	0.30
Level 5 80.00%	400.0	400.0	0.00	0.00
Remark : Measuring Range	500.0 ppb	Average Difference (%)		0.49
:Acceptable Limit \pm 5%				

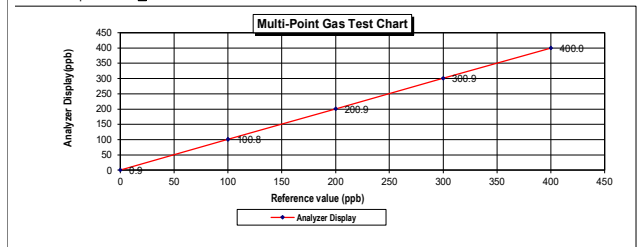

Calculate by *Smthan Cj*
15 / 05 / 2567

Approve by *Phrakhanong*
15 / May / 2024

CERTIFICATE OF ANALYSIS

Grade of Product: EPA PROTOCOL STANDARD

Customer: AIR LIQUIDE (THAILAND)
LTD--
Part Number: E05N191E15A0014
Cylinder Number: EB0162121
Laboratory: 124 - Plumsteadville - PA
PGVP Number: A12023
Gas Code: CO, CO₂, NO, NO₂, SO₂, BALN
Reference Number: 160-402772205-1
Cylinder Volume: 144.0 CF
Cylinder Pressure: 2015 PSIG
Valve Outlet: 660
Certification Date: Jul 06, 2023
Expiration Date: Jul 06, 2031

Certification performed in accordance with EPA Traceability Protocol for Assay and Certification of Gaseous Calibration Standards (May 2012) document EPA-820/R-02-051, using the assay procedures listed. Analytical Methodology does not require correction for analytical interference. This cylinder has a total analytical uncertainty as stated below with a confidence level of 95%. There are no significant impurities which affect the use of this calibration mixture. All concentrations are on a mole/mole basis unless otherwise noted. The results relate only to the items tested. The report shall not be reproduced except in full without approval of the laboratory. Do Not Use This Cylinder before 100 days, i.e. 3.7 months.

ANALYTICAL RESULTS					
Component	Requested Concentration	Actual Concentration	Protocol Method	Total Relative Uncertainty	Assay Dates
NOX	100.0 PPM	100.4 PPM	G1	\pm 0.9% NIST Traceable	06/27/2023, 07/06/2023
NITRIC OXIDE	100.0 PPM	100.2 PPM	G1	\pm 0.9% NIST Traceable	06/27/2023, 07/06/2023
SULFUR DIOXIDE	100.0 PPM	100.5 PPM	G1	\pm 1.4% NIST Traceable	06/27/2023, 07/06/2023
CARBON MONOXIDE	200.0 PPM	199.2 PPM	G1	\pm 0.3% NIST Traceable	06/26/2023
CARBON DIOXIDE	8,000 %	7,982 %	G1	\pm 1.3% NIST Traceable	06/27/2023
NITROGEN	Balance				

CALIBRATION STANDARDS					
Type	Lot ID	Cylinder No	Concentration	Uncertainty	Expiration Date
GMIS	104202308	CC754364	98.36 PPM NITRIC OXIDE/NITROGEN	\pm 0.4%	Jan 04, 2031
PRM	C2219101	AP15154048	100.16 PPM NITRIC OXIDE/NITROGEN	\pm 0.3%	Feb 28, 2025
GMIS	2023042525	CC754361	98.62 PPM NITRIC OXIDE/NITROGEN	\pm 0.4%	Apr 25, 2031
PRM	12459	D813880	15.01 PPM NITROGEN DIOXIDE/AIR	\pm 1.5%	Feb 17, 2023
GMIS	1534002092	EB0130037	9,893 PPM NITROGEN DIOXIDE/NITROGEN	\pm 1.0%	Sep 29, 2025
NTRM	160102-22	KAL203620	97.69 PPM SULFUR DIOXIDE/NITROGEN	\pm 0.9%	Nov 01, 2027
CO	230801	CC745902	249.47 PPM CARBON MONOXIDE/NITROGEN	\pm 0.3%	Dec 09, 2028
NTRM	130606-02	CCA11730	13.35% PPM CARBON DIOXIDE/NITROGEN	\pm 0.5%	May 14, 2025
The SRM, NTRM, PRM, or RSM noted above is only in reference to the GMIS used in the assay and not part of the analysis.					

ANALYTICAL EQUIPMENT		
Instrument/Make/Model	Analytical Principle	Last Multipoint Calibration
Nicolet iS65 FTIR AUP2010245 CO2	FTIR	Jun 15, 2023
SIEMENS ULTRAMATE 6E N1-CR-180	NDIR	Jun 14, 2023
Nicolet iS55 FTIR AUP2010245 NO	FTIR	Jun 29, 2023
Nicolet iS55 FTIR AUP2010245 NO2	FTIR	Jun 15, 2023
Nicolet iS55 FTIR AUP2010245 SO2	FTIR	Jun 08, 2023

Approved for Release



THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804, 0-2399-0469

Calibration Certificate

Issued by : Calibration & Test Section : Meteorological Instruments Bureau

Date of Issue : 22 February, 2024

Certification No. 099/24

Page : 1 of 5

Object : Wind Speed & Wind Direction Data Logger

Manufacturer : SCARLET/TECH

Type : WL-21

Mfg Code : Wireless Receiver 2205DR0114

Wind Sensor 2205DT0114

Customer : United Analyst and Engineering Consultant Co.,Ltd.

81 Soi Udomsuk 41, Sukhumvit Road,

Bangchak, Prakenong, Bangkok 10260.

Calibration Condition : Temperature 25.1 °C Barometric Pressure 1009.1 hPa

NATIONAL STANDARD WIND TUNNEL : Wind Afloat Plotting Board

: Micromanometer Theodor Friedrichs FC014 Serial No. 9310119 : HOOK GAGE NO 1425

N.I.S.T. Test Reference Number 731/241460 : Standard Velocity at 20 - 30 m/sec

: Ultrasonic Anemometer Model DA-650-3TV (sensor TR-90AH)

Serial Number 110730029 (sensor 120629586)

JAPAN QUALITY ASSURANCE ORGANIZATION : Standard Velocity at 0 - 20 m/sec

STANDARD THERMOMETER : Theodor Friedrich : Dry No.8390/94 Wet No. 8389/94

: testo, testo 645 Serial No. 02848057 : ThermoSchneider No.918802

STANDARD BAROMETER : Digital Barometer Vaisala Type PTB220 No. V1220015

: Digital Barometer Vaisala Type P19330 No. P19320001

Calibrated by : Watcharapol

Signed : Mr. Pibool Promsat

(Authorized Signatory)

for the Chief

Mr. Watcharapol Subwat

Mr. Pibool Promsat

Sub-Standard Instrument

Mechanical Engineer

เอกสารไม่ควบคุม



THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804, 0-2399-0469

The Result of Calibration

22 February, 2024

Certification No. 099/24

Page : 2 of 5

Standard	HOOK GAGE NO. 1425			TESTED ANEMOMETER	
	Pressure	Vacuum	Velocity	Velocity	Correction
Ultrasonic Anemometer	m/sec	mmHg H2O	mmHg H2O	m/sec	m/sec
1.00	-	-	-	1.0	0.00
3.02	-	-	-	3.0	0.02
5.00	-	-	-	5.0	0.00
7.04	-	-	-	7.0	0.04
9.02	-	-	-	9.0	0.02
11.02	-	-	-	11.0	0.02
13.01	-	-	-	13.0	0.01
15.01	-	-	-	15.0	0.01
17.02	-	-	-	17.0	0.02
20.02	-	-	-	20.0	0.02

Wind Afloat Plotting Board.	
US.DEPARTMENT OF COMMERCE WEATHER BUREAU	
WIND DIRECTION	TESTED WIND DIRECTION
0	0
90	90
180	180
270	270

Calibrated by :

Watcharapol

Mr. Watcharapol Subwat

Mechanical Engineer

Calibration & Test Section

Meteorological Instruments Bureau

เอกสารไม่ควบคุม



THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804, 0-2399-0469

The Result of Calibration

22 February, 2024

Certification No. 099/24

Page : 3 of 5

Standard Barometer	Tested Barometer	Correction
Pressure	Pressure	mmHg
1010.84	1011	-0.16
1010.60	1011	-0.40
1011.71	1012	-0.29
1012.17	1012	0.17
1012.31	1012	0.31
1012.25	1012	0.25
1012.79	1013	-0.21
1012.95	1013	-0.05
1013.52	1014	-0.48
1014.16	1014	0.16
1015.79	1016	-0.21
1016.02	1016	0.02
1015.86	1016	-0.14
1015.69	1016	-0.31
1011.51	1011	0.51
1011.60	1012	-0.20
1012.06	1012	0.06
1012.81	1013	-0.19
1013.22	1013	0.22
1013.49	1013	0.49

Average

-0.02

Calibrated by : Watcharapol

Mr. Watcharapol Subwat

Mechanical Engineer

Calibration & Test Section

Meteorological Instruments Bureau

เอกสารไม่ควบคุม



THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804, 0-2399-0469

The Result of Calibration

22 February, 2024

Certification No. 099/24

Page : 4 of 5

Standard Barometer	Tested Barometer	Correction
Pressure	Pressure	mmHg
756.19	758	0.19
758.01	758	0.01
758.64	759	-0.16
759.19	759	0.19
759.29	760	0.29
759.25	759	0.25
759.65	760	-0.35
758.77	760	-0.23
760.20	760	0.20
760.68	761	-0.32
761.90	762	-0.10
762.06	762	0.06
761.96	762	-0.04
761.83	762	-0.17
758.09	758	0.09
758.91	759	-0.09
759.11	759	0.11
759.67	760	-0.33
759.96	760	-0.02
760.16	760	0.16

Average

0.02

Calibrated by : Watcharapol

Mr. Watcharapol Subwat

Mechanical Engineer

Calibration & Test Section

Meteorological Instruments Bureau

เอกสารไม่ควบคุม



THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804, 0-2399-0469

The Result of Calibration

Certification No. 999/24

22 February, 2024

Page : 5 of 5

Standard Temp. °C	Temperature Sensor Reading	
	Reading °C	Correction °C
45.2	45	0.2
30.3	31	-0.7
15.8	16	-0.2

Calibrated by :

Handwritten signature

Mr. Watcharapol Subwat
Mechanical Engineer



เอกสารไม่ควบคุม

Certificate of Calibration

Customer

Name : UNITED ANALYST AND ENGINEERING
CONSULTANT CO.,LTD.
Address : 81 Soi Udomsak 41, Sukhumvit Road, Bangchak,
Prakanong, Bangkok 10260

Certificate No : 24-ACT-091
Request No : Req-2024-1380

Unit Under Calibration Details

Measurement item : Acoustic Calibrator
Manufacturer : SVANTEK
Model : SV 36
Serial Number : 107224
ID : UAE-EFM-171/2564
Class : 1
Range : 94 , 114 dB / 1000 Hz
Instrument Status : Used

Calibration Environment and Details

Temperature : (23 ±2 °C)
Humidity : (50 ± 20 %RH)
Barometric Pressure : (1013 ±10.0 hPa)
Received Date : 24 June 2024
Calibration Date : 26 June 2024
Location of Calibration : LAB 1 Acoustic
Calibration Procedure : In-house method CP-ACT-02 based on IEC 60942:2017 Electroacoustics - Sound calibrators

Reference Standard	Model	Serial Number	Traceable	Due Calibration
Sound Calibrator	SV 35A	58079	EEI	12 June 2025
THD Multimeter	2015	1047765	NIMT	16 January 2025

Traceability

This certificate provides traceability of measurement to recognized national standard, and to the realization of the international System of Units (SI).

Note

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor $k=2$, providing a level of confidence approximately 95 %.

Calibrated By :

Handwritten signature
Mr. Noppadon Luangart
Service Calibration Engineer

Approved By :

Handwritten signature
Mr. Pacit Mathavorn
Calibration Engineer Supervisor

Issue Date : 26 June 2024

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the laboratory.
เอกสารไม่ควบคุม

ISO 17025:2017 Rev 03 Issue date 5/6/24

Certificate No : 24-ACT-091

Request No : Req-2024-1380

Sound pressure level

Calibration Results : Without Adjustment

Calibration Range (dB)	Without Adjustment (dB)		Adjustment (dB)		Uncertainty (± dB)	Acceptance limit Class 1 (± dB)	Result
	Measured	Deviated value	Measured	Deviated value			
94 dB / 1000 Hz	94.02	0.02	-	-	0.14	0.25	Pass
114 dB / 1000 Hz	114.05	0.05	-	-	0.13	0.25	Pass

Frequency of Sound pressure level

Calibration Range (Hz)	Without Adjustment		Adjustment		Uncertainty (± %)	Acceptance limit Class 1 (± %)	Result
	Measured (Hz)	Deviated	Measured (Hz)	Deviated			
94 dB / 1000 Hz	1000.00	0.00	-	-	0.01	0.70	Pass
114 dB / 1000 Hz	1000.00	0.00	-	-	0.01	0.70	Pass

Total Harmonic Distortion plus Noise of Sound pressure level (THD+N %)

Calibration Range (Hz)	Without Adjustment	Adjustment	Uncertainty (± %)	Acceptance limit Class 1 (± %)	Result
	Measured (%)	Measured (%)			
94 dB / 1000 Hz	0.24	-	0.40	2.5	Pass
114 dB / 1000 Hz	0.44	-	0.40	2.5	Pass

Note :

Function	Maximum-permitted Uncertainty of measurement
Sound pressure level	0.15 dB
Frequency	0.20%
Total distortion+noise	0.50%

- Acceptance limit was IEC60942:2017 Class 1

- The calibration results exclude the calibrator pressure correction

- The calibration results exclude the microphone volume correction

เอกสารไม่ควบคุม

Certificate No : 24-ACT-091

Request No : Req-2024-1380

Decision Rule for Statements of Conformity


The standard decision rule employed for the statements of conformity to each calibration result will be applied using ILAC-G8:08:2019, Guidelines on the Reporting of Compliance with Specification as following Fig. and statements

Pass - The measurement result plus the expanded uncertainty with a 95% coverage probability were within the limit.

Pass¹ - The measurement result was within the limit. However, a portion of the expanded uncertainty of measurement at 95% exceeds the limit.

Fail² - The measurement result was out of the limit. However, a portion of the expanded uncertainty of measurement at 95% is within the limit.

Fail - The measurement result plus the expanded uncertainty with a 95% coverage probability were outside the limit.

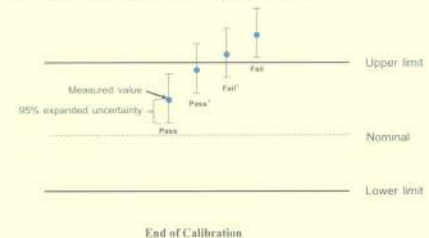

End of Calibration

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the laboratory.
เอกสารไม่ควบคุม

ISO 17025:2017 Rev 03 Issue date 5/6/24



ELECTRICAL AND ELECTRONICS INSTITUTE FOUNDATION FOR INDUSTRIAL DEVELOPMENT

975 Moo 4, Bangpoo Industrial Estate, Soi 8, Sukhumvit Road km 37,
Phraek Sa, Mueang Samut Prakan, Samut Prakan 10280
Tel: +66 2709 4860 Fax: +66 2324 0917



Certificate No.: CP20240323EA
Operation No.: CP2024080294

Certificate of Calibration

Equipment: Sound Level Meter

Manufacturer: Larson Davis (Meter), PCB (Microphone), PCB (Preamplifier)

Model/Type: LxT1 (Meter), 377B02 (Microphone), PRMLxT1 (Preamplifier)

Serial No.: 0007305 (Meter), 345234 (Microphone), 077640 (Preamplifier)

ID No.: UAE.EFM.038/2566

Customer: United Analyst and Engineering Consultant Co.,Ltd.

Address: 81 Soi Udomsuk 41, Sukhumvit Road, Bangchak
Phrakhanong, Bangkok 10260

Received Date: 9 August 2024

Calibrated Date: 22 - 27 August 2024

Issued Date: 28 August 2024

Calibrated by: Ms. Juntaporn Kunhakom

Approved by: 
(Mr. Sittichai Swaksuriyawong)
Group Manager

This report was prepared electronically using applicable electronic signature. Printing or copy of file are considered as a copy of the document.

The reported uncertainty of measurement was based on standard uncertainty multiplied by a coverage factor (k) providing a level of confidence of approximately 95%. This certificate may not be reproduced other than in full except with the prior written approval of the Electrical and Electronics Institute, Foundation for Industrial Development.

Page 1 of 6

เอกสารไม่ควบคุม

F-CAL-004 Ed.1



ELECTRICAL AND ELECTRONICS INSTITUTE FOUNDATION FOR INDUSTRIAL DEVELOPMENT

Certificate No.: CP20240323EA

Calibration Report

Equipment: Sound Level Meter

Manufacturer: Larson Davis (Meter), PCB (Microphone), PCB (Preamplifier)

Model/Type: LxT1 (Meter), 377B02 (Microphone), PRMLxT1 (Preamplifier)

Serial No.: 0007305 (Meter), 345234 (Microphone), 077640 (Preamplifier)

ID No.: UAE.EFM.038/2566

Ambient Temperature: (23 ± 2) °C

Relative Humidity: (50 ± 15) %

Pressure: (101.3 ± 1.5) kPa

Method of Calibration :-
IEC 61672-3:2013.

Condition of this result of calibration

1. Reference standards instrument :-

Instrument	Model	Serial No.	Cert. No.	Due Date
1) Standard microphone	4180	2787490	AA-1012-23	12 November 2024
2) Arbitrary Function Generator	AFG2021	C010063	CK20240048EA	23 June 2025
3) Programmable Attenuator	PA5	2755	EF-0040-23	1 October 2024
4) 6.5 Digit precision multimeter	8846A	9610014	CB20230200EA	15 November 2024
5) Pressure humidity and Temperature Transmitter	PTU301	L3950483	CL1-P240023 CD20240142EA	24 March 2025 12 June 2025
6) Pressure humidity and Temperature Transmitter	PTU301	L3950484	CL1-P240030 CD20240143EA	11 April 2025 12 June 2025
7) Performance Audio Analyzer	U8903B	MY56510003	CB20240035EB CK20230072EA	13 February 2025 13 September 2024

2. This result of calibration was found accurate as shown on date and place of calibration only.

3. This certification is traceable to the international system of unit maintained at :-

Reference standards instrument for Acoustic function

- National Institute of Metrology (Thailand)

Reference standards instrument for Electrical function

- National Institute of Metrology (Thailand)

- Electrical and Electronics Institute; NSC Accredited Calibration No.0119

Result of Calibration:-

Function : 1. Indication at the calibration check frequency

Reference Acoustic Signal (dB)	Measured value (dB)	Deviation (dB)	Acceptance limits (dB)
-	-	-	-

Page 2 of 6

F-CAL-005 Ed.1

เอกสารไม่ควบคุม



ELECTRICAL AND ELECTRONICS INSTITUTE FOUNDATION FOR INDUSTRIAL DEVELOPMENT

Certificate No.: CP20240323EA

Calibration Report

Function : 2. Self-generated Noise

2.1 Microphone Installed

Measured value (dB)
30.1

2.2 Microphone replaced by the electrical input signal device

Frequency Weighting	Measured value (dB)
A-weighting	29.9
C-weighting	30.0
Z-weighting	35.5

Function : 3. Acoustical signal tests of frequency weightings (Without Windscreen)

Meter free-field acoustic response at a level of 84 dB.

Frequency (Hz)	Deviation from various Frequency Weighting Response Curve			
	C-Weighting (dB)	A-Weighting (dB)	Z-Weighting (dB)	Acceptance limits (dB)
125	0.2	0.1	0.1	±1.0
1000	-0.1	-0.1	-0.1	±0.7
8000	0.6	0.5	0.6	+1.5; -2.5

Function : 4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various Frequency Weighting Response Curve			
	C-Weighting (dB)	A-Weighting (dB)	Z-Weighting (dB)	Acceptance limits (dB)
63	0.0	-0.1	0.0	±1.0
125	0.0	-0.1	0.0	±1.0
250	0.0	-0.1	0.0	±1.0
500	0.0	-0.1	0.0	±1.0
1000	0.0	0.0	0.0	±0.7
2000	0.0	-0.1	0.0	±1.0
4000	0.0	-0.1	0.0	±1.0
8000	-0.1	-0.1	0.0	+1.5; -2.5
16000	0.0	0.0	0.0	+2.5; -16.0

เอกสารไม่ควบคุม

Page 3 of 6

F-CAL-005 Ed.1



ELECTRICAL AND ELECTRONICS INSTITUTE FOUNDATION FOR INDUSTRIAL DEVELOPMENT

Certificate No.: CP20240323EA

Calibration Report

Function : 5. Frequency and time weighting at 1 kHz

5.1 Frequency weighting at 1 kHz

Frequency Weighting	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
C-weighting	94.0	0.0	±0.2
A-weighting	94.0	0.0	±0.2
Z-weighting	94.0	0.0	±0.2

5.2 Time weighting at 1 kHz

Time Weighting	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
Fast	94.0	0.0	±0.1
Slow	94.0	0.0	±0.1
LAeq	94.0	0.0	±0.1

Function : 6. Long-Term Stability

Long-term stability over 30 minutes, with steady 1 kHz signal at reference level.

Time Period to Apply Signal (min)	Reference SPL (dB)	Record SPL at Conclusion of Time Period (dB)	Deviated value (dB)	Acceptance limits (dB)
30	94.0	94.0	0.0	±0.1

Function : 7. Level Linearity on the reference level range

7.1 Level Linearity on the reference level range, Upper

Anticipated Value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
94.0	94.0	0.0	±0.8
99.0	99.0	0.0	±0.8
104.0	104.0	0.0	±0.8
109.0	109.0	0.0	±0.8
114.0	114.0	0.0	±0.8
119.0	119.0	0.0	±0.8
124.0	124.0	0.0	±0.8
129.0	129.0	0.0	±0.8
134.0	134.0	0.0	±0.8
139.0	139.0	0.0	±0.8
140.0	140.0	0.0	±0.8
141.0	141.0	0.0	±0.8

เอกสารไม่ควบคุม

Page 4 of 6

F-CAL-005 Ed.1

Certificate No.: CP20240323EA

Calibration Report

7.2 Level Linearity on the reference level range, Lower

Anticipated Value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
94.0	94.0	0.0	±0.8
89.0	89.0	0.0	±0.8
84.0	84.0	0.0	±0.8
79.0	79.0	0.0	±0.8
74.0	74.0	0.0	±0.8
69.0	69.0	0.0	±0.8
64.0	64.0	0.0	±0.8
59.0	59.0	0.0	±0.8
54.0	54.0	0.0	±0.8
49.0	49.0	0.0	±0.8
44.0	44.1	0.1	±0.8
39.0	39.4	0.4	±0.8

Function : 8. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
Fast	200	136.0	0.0	±0.5
	2	118.9	-0.1	+1.0 ; -1.5
	0.25	109.7	-0.3	+1.0 ; -3.0
Slow	200	129.5	-0.1	±0.5
	2	109.9	-0.1	+1.0 ; -3.0
	200	130.0	0.0	±0.5
LAE	2	110.0	0.0	+1.0 ; -1.5
	0.25	100.9	-0.1	+1.0 ; -3.0

Function : 9. Peak C sound level

Number of cycles in test signal	Anticipated Value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
Complete cycle	135.4	134.8	-0.6	±2.0
Positive half cycle	134.4	134.0	-0.4	±1.0
Negative half cycle	134.4	134.0	-0.4	±1.0

Page 5 of 6

F-CAL-005 Ed.1

เอกสารไม่ควบคุม

Certificate No.: CP20240323EA

Calibration Report

Function : 10. Overload indication

Measured value (dB)		Deviated value (dB)	Acceptance limits (dB)
Positive one-half cycle	Negative one-half cycle		
143.7	143.7	0.0	±1.5

Function : 11. High-Level Stability

High-level stability over 5 minutes, with steady 1 kHz signal, 1 dB below upper boundary.

Time Period to Apply Signal (min)	Reference SPL (dB)	Record SPL at Conclusion of Time Period (dB)	Deviated value (dB)	Acceptance limits (dB)
5	139.0	139.0	0.0	±0.1

Uncertainty of measurement

Function	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1) Indication at the calibration check frequency	0.30	Not applicable
2) Self-generated Noise	0.10	Not applicable
3) Acoustical signal tests of frequency weightings - Free-field sound pressure response level	0.30	0.60 (10Hz to 4kHz) 0.70 (>4kHz to 10kHz)
4) Electrical signal tests of frequency weightings	0.20	0.20
5) Frequency and time weighting at 1 kHz	0.20	0.20
6) Long-Term Stability	0.10	0.10
7) Level Linearity on the reference level range	0.30	0.30
8) Tone burst response	0.20	0.30
9) Peak C sound level	0.20	0.35
10) Overload indication	0.20	0.25
11) High-Level Stability	0.10	0.10

Remarks:

1. Indication at the calibration check frequency can not measured because customer does not provide a sound calibrator.
2. The acceptance limit is for the deviated value.
3. Acceptance limits was IEC61672-3:2013 Class 1.
4. The coverage factor $k = 2.00$

- - End of Report - -

Page 6 of 6

F-CAL-005 Ed.1

เอกสารไม่ควบคุม

Certificate No.: CP20240290EA

Operation No.: CP2024070253

Certificate of Calibration

Equipment: Sound Level Meter

Manufacturer: Larson Davis (Meter), PCB (Microphone), PCB (Preamplifier)

Model/Type: LxT1 (Meter), 377B02 (Microphone), PRMLxT1 (Preamplifier)

Serial No.: 0007306 (Meter), 345235 (Microphone), 077641 (Preamplifier)

ID No.: UAE.EFM.039/2566

Customer: United Analyst and Engineering Consultant Co.,Ltd.

Address: 81 Soi Udomsuk 41, Sukhumvit Road, Bangchak Phrakhanong, Bangkok 10260

Received Date: 25 July 2024

Calibrated Date: 5 - 6 August 2024

Issued Date: 7 August 2024

Calibrated by: Ms. Juntaporn Kunhakom

Approved by:

(Mr. Sittichai Swaksuriyawong)
Group Manager

This report was prepared electronically using applicable electronic signature. Printing or copy of file are considered as a copy of the document.

The reported uncertainty of measurement was based on standard uncertainty multiplied by a coverage factor (k) providing a level of confidence of approximately 95%. This certificate may not be reproduced other than in full except with the prior written approval of the Electrical and Electronics Institute, Foundation for Industrial Development.

Page 1 of 6

เอกสารไม่ควบคุม

F-CAL-004 Ed.1

Certificate No.: CP20240290EA

Calibration Report

Equipment: Sound Level Meter

Manufacturer: Larson Davis (Meter), PCB (Microphone), PCB (Preamplifier)

Model/Type: LxT1 (Meter), 377B02 (Microphone), PRMLxT1 (Preamplifier)

Serial No.: 0007306 (Meter), 345235 (Microphone), 077641 (Preamplifier)

ID No.: UAE.EFM.039/2566

Ambient Temperature: (23 ± 2) °C

Relative Humidity: (50 ± 15) %

Pressure: (101.3 ± 1.5) kPa

Method of Calibration :- IEC 61672-3:2013.

Condition of this result of calibration

1. Reference standards instrument :-

Instrument	Model	Serial No.	Cert. No.	Due Date
1) Standard microphone	4180	2787490	AA-1012-23	12 November 2024
2) Arbitrary Function Generator	AFG2021	C010063	CK20240048EA	23 June 2025
3) Programmable Attenuator	PA5	2755	EF-0040-23	1 October 2024
4) 6.5 Digit precision multimeter	8846A	9610014	CB20230200EA	15 November 2024
5) Pressure humidity and Temperature Transmitter	PTU301	L3950483	CL1-P240023 CD20240142EA	24 March 2025 12 June 2025
6) Pressure humidity and Temperature Transmitter	PTU301	L3950484	CL1-P240030 CD20240143EA	11 April 2025 12 June 2025
7) Performance Audio Analyzer	U8903B	MY56510003	CB20240035EB CK20230072EA	13 February 2025 13 September 2024

2. This result of calibration was found accurate as shown on date and place of calibration only.

3. This certification is traceable to the international system of unit maintained at :-

Reference standards instrument for Acoustic function

- National Institute of Metrology (Thailand)

Reference standards instrument for Electrical function

- National Institute of Metrology (Thailand)
- Electrical and Electronics Institute; NSC Accredited Calibration No.0119

Result of Calibration:-

Function : 1. Indication at the calibration check frequency

Reference Acoustic Signal (dB)	Measured value (dB)	Deviation (dB)	Acceptance limits (dB)
-	-	-	-

Page 2 of 6

F-CAL-005 Ed.1

เอกสารไม่ควบคุม

Certificate No.: CP20240290EA

Calibration Report

Function : 2. Self-generated Noise

2.1 Microphone Installed

Measured value (dB)
28.8

2.2 Microphone replaced by the electrical input signal device

Frequency Weighting	Measured value (dB)
A-weighting	28.7
C-weighting	28.4
Z-weighting	34.5

Function : 3. Acoustical signal tests of frequency weightings (Without Windscreen)

Meter free-field acoustic response at a level of 84 dB.

Frequency (Hz)	Deviation from various Frequency Weighting Response Curve			
	C-Weighting (dB)	A-Weighting (dB)	Z-Weighting (dB)	Acceptance limits (dB)
125	0.1	0.0	0.0	±1.0
1000	-0.1	-0.1	-0.1	±0.7
8000	-0.4	-0.5	-0.4	+1.5; -2.5

Function : 4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various Frequency Weighting Response Curve			
	C-Weighting (dB)	A-Weighting (dB)	Z-Weighting (dB)	Acceptance limits (dB)
63	0.0	0.0	0.0	±0.8
125	0.0	0.0	0.0	±1.0
250	0.0	0.0	0.0	±1.0
500	0.0	0.0	0.0	±1.0
1000	0.0	0.0	0.0	±0.7
2000	0.0	0.0	0.0	±1.0
4000	0.0	0.0	0.0	±1.0
8000	-0.1	-0.1	0.0	+1.5; -2.5
16000	0.0	0.0	0.0	+2.5; -16.0

เอกสารไม่ควบคุม

Page 3 of 6

F-CAL-005 Ed.1

Certificate No.: CP20240290EA

Calibration Report

Function : 5. Frequency and time weighting at 1 kHz

5.1 Frequency weighting at 1 kHz

Frequency Weighting	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
C-weighting	94.0	0.0	±0.2
A-weighting	94.0	0.0	±0.2
Z-weighting	94.0	0.0	±0.2

5.2 Time weighting at 1 kHz

Time Weighting	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
Fast	94.0	0.0	±0.1
Slow	94.0	0.0	±0.1
LAeq	94.0	0.0	±0.1

Function : 6. Long-Term Stability

Long-term stability over 30 minutes, with steady 1 kHz signal at reference level.

Time Period to Apply Signal (min)	Reference SPL (dB)	Record SPL at Conclusion of Time Period (dB)	Deviated value (dB)	Acceptance limits (dB)
30	94.0	94.0	0.0	±0.1

Function : 7. Level Linearity on the reference level range

7.1 Level Linearity on the reference level range, Upper

Anticipated Value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
94.0	94.0	0.0	±0.8
99.0	99.0	0.0	±0.8
104.0	104.0	0.0	±0.8
109.0	109.0	0.0	±0.8
114.0	114.0	0.0	±0.8
119.0	119.0	0.0	±0.8
124.0	124.0	0.0	±0.8
129.0	129.0	0.0	±0.8
134.0	134.0	0.0	±0.8
139.0	139.0	0.0	±0.8
140.0	140.0	0.0	±0.8

เอกสารไม่ควบคุม

Page 4 of 6

F-CAL-005 Ed.1

Certificate No.: CP20240290EA

Calibration Report

7.2 Level Linearity on the reference level range, Lower

Anticipated Value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
94.0	94.0	0.0	±0.8
89.0	89.0	0.0	±0.8
84.0	84.0	0.0	±0.8
79.0	79.0	0.0	±0.8
74.0	74.0	0.0	±0.8
69.0	69.0	0.0	±0.8
64.0	64.0	0.0	±0.8
59.0	59.0	0.0	±0.8
54.0	54.0	0.0	±0.8
49.0	49.0	0.0	±0.8
44.0	44.1	0.1	±0.8
39.0	39.4	0.4	±0.8

Function : 8. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
Fast	200	136.0	0.0	±0.5
	2	118.8	-0.2	+1.0 ; -1.5
	0.25	109.7	-0.3	+1.0 ; -3.0
Slow	200	129.5	-0.1	±0.5
	2	109.8	-0.2	+1.0 ; -3.0
	200	130.0	0.0	±0.5
LAE	2	110.0	0.0	+1.0 ; -1.5
	0.25	100.9	-0.1	+1.0 ; -3.0

Function : 9. Peak C sound level

Number of cycles in test signal	Anticipated Value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
Complete cycle	135.4	134.8	-0.6	±2.0
Positive half cycle	134.4	134.0	-0.4	±1.0
Negative half cycle	134.4	134.0	-0.4	±1.0

เอกสารไม่ควบคุม

Page 5 of 6

F-CAL-005 Ed.1

Certificate No.: CP20240290EA

Calibration Report

Function : 10. Overload indication

Measured value (dB)		Deviated value (dB)	Acceptance limits (dB)
Positive one-half cycle	Negative one-half cycle		
142.6	142.6	0.0	±1.5

Function : 11. High-Level Stability

High-level stability over 5 minutes, with steady 1 kHz signal, 1 dB below upper boundary.

Time Period to Apply Signal (min)	Reference SPL (dB)	Record SPL at Conclusion of Time Period (dB)	Deviated value (dB)	Acceptance limits (dB)
5	139.0	139.0	0.0	±0.1

Uncertainty of measurement

Function	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1) Indication at the calibration check frequency	0.30	Not applicable
2) Self-generated Noise	0.10	Not applicable
3) Acoustical signal tests of frequency weightings - Free-field sound pressure response level	0.30	0.60 (10Hz to 4kHz) 0.70 (>4kHz to 10kHz)
4) Electrical signal tests of frequency weightings	0.20	0.20
5) Frequency and time weighting at 1 kHz	0.20	0.20
6) Long-Term Stability	0.10	0.10
7) Level Linearity on the reference level range	0.30	0.30
8) Tone burst response	0.20	0.30
9) Peak C sound level	0.20	0.35
10) Overload indication	0.20	0.25
11) High-Level Stability	0.10	0.10

Remarks:

1. Indication at the calibration check frequency can not measured because customer does not provide a sound calibrator.
2. The acceptance limit is for the deviated value.
3. Acceptance limits was IEC61672-3:2013 Class 1.
4. The coverage factor $k = 2.00$

- - End of Report - -

เอกสารไม่ควบคุม

Page 6 of 6

F-CAL-005 Ed.1



ELECTRICAL AND ELECTRONICS INSTITUTE FOUNDATION FOR INDUSTRIAL DEVELOPMENT

975 Moo 4, Bangpoo Industrial Estate, Soi 8, Sukhumvit Road km 37,
Phraek Sa, Mueang Samut Prakan, Samut Prakan 10280
Tel: +66 2709 4860 Fax: +66 2324 0917



Certificate No.: CP20240322EA
Operation No.: CP2024080293

Certificate of Calibration

Equipment: Sound Level Meter

Manufacturer: Larson Davis (Meter), PCB (Microphone), PCB (Preamplifier)

Model/Type: LxT1 (Meter), 377B02 (Microphone), PRMLxT1 (Preamplifier)

Serial No.: 0007308 (Meter), 345238 (Microphone), 077643 (Preamplifier)

ID No.: UAE.EFM.040/2566

Customer: United Analyst and Engineering Consultant Co.,Ltd.


Address: 81 Soi Udomsuk 41, Sukhumvit Road, Bangchak
Phrakhanong, Bangkok 10260

Received Date: 9 August 2024

Calibrated Date: 22 - 26 August 2024

Issued Date: 28 August 2024

Calibrated by: Ms. Juntaporn Kunhakom

Approved by: 
(Mr. Sittichai Swaksuriyawong)
Group Manager

This report was prepared electronically using applicable electronic signature. Printing or copy of file are considered as a copy of the document.

The reported uncertainty of measurement was based on standard uncertainty multiplied by a coverage factor (k) providing a level of confidence of approximately 95%. This certificate may not be reproduced other than in full except with the prior written approval of the Electrical and Electronics Institute, Foundation for Industrial Development.

Page 1 of 6

เอกสารไม่ควบคุม

F-CAL-004 Ed.1



ELECTRICAL AND ELECTRONICS INSTITUTE FOUNDATION FOR INDUSTRIAL DEVELOPMENT

Certificate No.: CP20240322EA

Calibration Report

Equipment: Sound Level Meter

Manufacturer: Larson Davis (Meter), PCB (Microphone), PCB (Preamplifier)

Model/Type: LxT1 (Meter), 377B02 (Microphone), PRMLxT1 (Preamplifier)

Serial No.: 0007308 (Meter), 345238 (Microphone), 077643 (Preamplifier)

ID No.: UAE.EFM.040/2566

Ambient Temperature: (23 ± 2) °C

Relative Humidity: (50 ± 15) %

Pressure: (101.3 ± 1.5) kPa

Method of Calibration :-
IEC 61672-3:2013.

Condition of this result of calibration

1. Reference standards instrument :-

Instrument	Model	Serial No.	Cert. No.	Due Date
1) Standard microphone	4180	2787490	AA-1012-23	12 November 2024
2) Arbitrary Function Generator	AFG2021	C010063	CK20240048EA	23 June 2025
3) Programmable Attenuator	PA5	2755	EF-0040-23	1 October 2024
4) 6.5 Digit precision multimeter	8846A	9610014	CB20230200EA	15 November 2024
5) Pressure humidity and Temperature Transmitter	PTU301	L3950483	CL1-P240023 CD20240142EA	24 March 2025 12 June 2025
6) Pressure humidity and Temperature Transmitter	PTU301	L3950484	CL1-P240030 CD20240143EA	11 April 2025 12 June 2025
7) Performance Audio Analyzer	U8903B	MY56510003	CB20240035EB CK20230072EA	13 February 2025 13 September 2024

2. This result of calibration was found accurate as shown on date and place of calibration only.

3. This certification is traceable to the international system of unit maintained at :-

Reference standards instrument for Acoustic function

- National Institute of Metrology (Thailand)

Reference standards instrument for Electrical function

- National Institute of Metrology (Thailand)

- Electrical and Electronics Institute; NSC Accredited Calibration No.0119

Result of Calibration:-

Function : 1. Indication at the calibration check frequency

Reference Acoustic Signal (dB)	Measured value (dB)	Deviation (dB)	Acceptance limits (dB)
-	-	-	-

Page 2 of 6

F-CAL-005 Ed.1

เอกสารไม่ควบคุม



ELECTRICAL AND ELECTRONICS INSTITUTE FOUNDATION FOR INDUSTRIAL DEVELOPMENT

Certificate No.: CP20240322EA

Calibration Report

Function : 2. Self-generated Noise

2.1 Microphone Installed

Measured value (dB)
29.4

2.2 Microphone replaced by the electrical input signal device

Frequency Weighting	Measured value (dB)
A-weighting	29.0
C-weighting	28.9
Z-weighting	35.5

Function : 3. Acoustical signal tests of frequency weightings (Without Windscreen)

Meter free-field acoustic response at a level of 84 dB.

Frequency (Hz)	Deviation from various Frequency Weighting Response Curve			
	C-Weighting (dB)	A-Weighting (dB)	Z-Weighting (dB)	Acceptance limits (dB)
125	0.2	0.1	0.2	±1.0
1000	0.3	0.3	0.3	±0.7
8000	-0.6	-0.5	-0.5	+1.5; -2.5

Function : 4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various Frequency Weighting Response Curve			
	C-Weighting (dB)	A-Weighting (dB)	Z-Weighting (dB)	Acceptance limits (dB)
63	-0.1	0.1	0.0	±1.0
125	0.0	0.0	-0.1	±1.0
250	-0.1	0.0	0.0	±1.0
500	0.0	0.0	-0.1	±1.0
1000	0.0	0.0	0.0	±0.7
2000	0.0	0.0	0.0	±1.0
4000	0.0	-0.1	0.0	±1.0
8000	-0.1	-0.1	0.0	+1.5; -2.5
16000	0.0	0.0	-0.1	+2.5; -16.0

เอกสารไม่ควบคุม

Page 3 of 6

F-CAL-005 Ed.1



ELECTRICAL AND ELECTRONICS INSTITUTE FOUNDATION FOR INDUSTRIAL DEVELOPMENT

Certificate No.: CP20240322EA

Calibration Report

Function : 5. Frequency and time weighting at 1 kHz

5.1 Frequency weighting at 1 kHz

Frequency Weighting	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
C-weighting	94.0	0.0	±0.2
A-weighting	94.0	0.0	±0.2
Z-weighting	94.0	0.0	±0.2

5.2 Time weighting at 1 kHz

Time Weighting	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
Fast	94.0	0.0	±0.1
Slow	94.0	0.0	±0.1
LAeq	94.0	0.0	±0.1

Function : 6. Long-Term Stability

Long-term stability over 30 minutes, with steady 1 kHz signal at reference level.

Time Period to Apply Signal (min)	Reference SPL (dB)	Record SPL at Conclusion of Time Period (dB)	Deviated value (dB)	Acceptance limits (dB)
30	94.0	94.0	0.0	±0.1

Function : 7. Level Linearity on the reference level range

7.1 Level Linearity on the reference level range, Upper

Anticipated Value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
94.0	94.0	0.0	±0.8
99.0	99.0	0.0	±0.8
104.0	104.0	0.0	±0.8
109.0	109.0	0.0	±0.8
114.0	114.0	0.0	±0.8
119.0	119.0	0.0	±0.8
124.0	124.0	0.0	±0.8
129.0	129.0	0.0	±0.8
134.0	134.0	0.0	±0.8
139.0	139.0	0.0	±0.8
140.0	140.0	0.0	±0.8

Page 4 of 6

F-CAL-005 Ed.1

เอกสารไม่ควบคุม

Certificate No.: CP20240322EA

Calibration Report

7.2 Level Linearity on the reference level range, Lower

Anticipated Value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
94.0	94.0	0.0	±0.8
89.0	89.0	0.0	±0.8
84.0	84.0	0.0	±0.8
79.0	79.0	0.0	±0.8
74.0	74.0	0.0	±0.8
69.0	69.0	0.0	±0.8
64.0	64.0	0.0	±0.8
59.0	59.0	0.0	±0.8
54.0	54.0	0.0	±0.8
49.0	49.0	0.0	±0.8
44.0	44.1	0.1	±0.8
39.0	39.4	0.4	±0.8

Function : 8. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
Fast	200	135.9	-0.1	±0.5
	2	118.8	-0.2	+1.0 ; -1.5
	0.25	109.6	-0.4	+1.0 ; -3.0
Slow	200	129.5	-0.1	±0.5
	2	109.8	-0.2	+1.0 ; -3.0
	200	130.0	0.0	±0.5
LAE	2	110.0	0.0	+1.0 ; -1.5
	0.25	100.8	-0.2	+1.0 ; -3.0

Function : 9. Peak C sound level

Number of cycles in test signal	Anticipated Value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
Complete cycle	135.4	134.8	-0.6	±2.0
Positive half cycle	134.4	134.0	-0.4	±1.0
Negative half cycle	134.4	134.1	-0.3	±1.0

Page 5 of 6

F-CAL-005 Ed.1

เอกสารไม่ควบคุม

Certificate No.: CP20240322EA

Calibration Report

Function : 10. Overload indication

Measured value (dB)		Deviated value (dB)	Acceptance limits (dB)
Positive one-half cycle	Negative one-half cycle		
143.0	142.8	-0.2	±1.5

Function : 11. High-Level Stability

High-level stability over 5 minutes, with steady 1 kHz signal, 1 dB below upper boundary.

Time Period to Apply Signal (min)	Reference SPL (dB)	Record SPL at Conclusion of Time Period (dB)	Deviated value (dB)	Acceptance limits (dB)
5	139.0	139.0	0.0	±0.1

Uncertainty of measurement

Function	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1) Indication at the calibration check frequency	0.30	Not applicable
2) Self-generated Noise	0.10	Not applicable
3) Acoustical signal tests of frequency weightings - Free-field sound pressure response level	0.30	0.60 (10Hz to 4kHz) 0.70 (>4kHz to 10kHz)
4) Electrical signal tests of frequency weightings	0.20	0.20
5) Frequency and time weighting at 1 kHz	0.20	0.20
6) Long-Term Stability	0.10	0.10
7) Level Linearity on the reference level range	0.30	0.30
8) Tone burst response	0.20	0.30
9) Peak C sound level	0.20	0.35
10) Overload indication	0.20	0.25
11) High-Level Stability	0.10	0.10

Remarks:

1. Indication at the calibration check frequency can not measured because customer does not provide a sound calibrator.
2. The acceptance limit is for the deviated value.
3. Acceptance limits was IEC61672-3:2013 Class 1.
4. The coverage factor $k = 2.00$

- - End of Report - -

Page 6 of 6

F-CAL-005 Ed.1

เอกสารไม่ควบคุม

Certificate No.: CP20240287EA
Operation No.: CP2024070250

Certificate of Calibration

Equipment: Sound Level Meter

Manufacturer: Larson Davis (Meter), PCB (Microphone), PCB (Preamplifier)

Model/Type: LxT1 (Meter), 377B02 (Microphone), PRMLxT1 (Preamplifier)

Serial No.: 0007309 (Meter), 345239 (Microphone), 077644 (Preamplifier)

ID No.: UAE.EFM.041/2566

Customer: United Analyst and Engineering Consultant Co.,Ltd.

Address: 81 Soi Udomsuk 41, Sukhumvit Road, Bangchak Phrakhanong, Bangkok 10260

Received Date: 25 July 2024

Calibrated Date: 2 - 5 August 2024

Issued Date: 7 August 2024

Calibrated by: Ms. Juntaporn Kunhakom

Approved by:

(Mr. Sittichai Swaksuriyawong)
Group Manager

This report was prepared electronically using applicable electronic signature. Printing or copy of file are considered as a copy of the document.

The reported uncertainty of measurement was based on standard uncertainty multiplied by a coverage factor (k) providing a level of confidence of approximately 95%. This certificate may not be reproduced other than in full except with the prior written approval of the Electrical and Electronics Institute, Foundation for Industrial Development.

Page 1 of 6

เอกสารไม่ควบคุม

F-CAL-004 Ed.1

Certificate No.: CP20240287EA

Calibration Report

Equipment: Sound Level Meter

Manufacturer: Larson Davis (Meter), PCB (Microphone), PCB (Preamplifier)

Model/Type: LxT1 (Meter), 377B02 (Microphone), PRMLxT1 (Preamplifier)

Serial No.: 0007309 (Meter), 345239 (Microphone), 077644 (Preamplifier)

ID No.: UAE.EFM.041/2566

Ambient Temperature: (23 ± 2) °C

Relative Humidity: (50 ± 15) %

Pressure: (101.3 ± 1.5) kPa

Method of Calibration :- IEC 61672-3:2013.

Condition of this result of calibration

1. Reference standards instrument :-

Instrument	Model	Serial No.	Cert. No.	Due Date
1) Standard microphone	4180	2787490	AA-1012-23	12 November 2024
2) Arbitrary Function Generator	AFG2021	C010063	CK20240048EA	23 June 2025
3) Programmable Attenuator	PA5	2755	EF-0040-23	1 October 2024
4) 6.5 Digit precision multimeter	8846A	9610014	CB20230200EA	15 November 2024
5) Pressure humidity and Temperature Transmitter	PTU301	L3950483	CL1-P240023 CD20240142EA	24 March 2025 12 June 2025
6) Pressure humidity and Temperature Transmitter	PTU301	L3950484	CL1-P240030 CD20240143EA	11 April 2025 12 June 2025
7) Performance Audio Analyzer	U8903B	MY56510003	CB20240035EB CK20230072EA	13 February 2025 13 September 2024

2. This result of calibration was found accurate as shown on date and place of calibration only.

3. This certification is traceable to the international system of unit maintained at :-

Reference standards instrument for Acoustic function

- National Institute of Metrology (Thailand)

Reference standards instrument for Electrical function

- National Institute of Metrology (Thailand)
- Electrical and Electronics Institute; NSC Accredited Calibration No.0119

Result of Calibration:-

Function : 1. Indication at the calibration check frequency

Reference Acoustic Signal (dB)	Measured value (dB)	Deviation (dB)	Acceptance limits (dB)
-	-	-	-

Page 2 of 6

F-CAL-005 Ed.1

เอกสารไม่ควบคุม

Certificate No.: CP20240287EA

Calibration Report

Function : 2. Self-generated Noise

2.1 Microphone Installed

Measured value (dB)
30.5

2.2 Microphone replaced by the electrical input signal device

Frequency Weighting	Measured value (dB)
A-weighting	29.5
C-weighting	29.5
Z-weighting	35.5

Function : 3. Acoustical signal tests of frequency weightings (Without Windscreen)

Meter free-field acoustic response at a level of 84 dB.

Frequency (Hz)	Deviation from various Frequency Weighting Response Curve			
	C-Weighting (dB)	A-Weighting (dB)	Z-Weighting (dB)	Acceptance limits (dB)
125	0.4	0.3	0.4	±1.0
1000	0.1	0.1	0.1	±0.7
8000	-1.6	-1.6	-1.6	+1.5; -2.5

Function : 4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various Frequency Weighting Response Curve			
	C-Weighting (dB)	A-Weighting (dB)	Z-Weighting (dB)	Acceptance limits (dB)
63	0.0	0.0	0.0	±0.8
125	0.0	0.0	-0.1	±1.0
250	0.0	0.0	-0.1	±1.0
500	0.0	0.0	-0.1	±1.0
1000	0.0	0.0	0.0	±0.7
2000	0.0	0.0	-0.1	±1.0
4000	0.0	0.0	-0.1	±1.0
8000	-0.1	-0.1	0.0	+1.5; -2.5
16000	0.0	0.0	-0.1	+2.5; -16.0

เอกสารไม่ควบคุม

Page 3 of 6

F-CAL-005 Ed.1

Certificate No.: CP20240287EA

Calibration Report

7.2 Level Linearity on the reference level range, Lower

Anticipated Value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
94.0	94.0	0.0	±0.8
89.0	89.0	0.0	±0.8
84.0	84.0	0.0	±0.8
79.0	79.0	0.0	±0.8
74.0	74.0	0.0	±0.8
69.0	69.0	0.0	±0.8
64.0	64.0	0.0	±0.8
59.0	59.0	0.0	±0.8
54.0	54.0	0.0	±0.8
49.0	49.0	0.0	±0.8
44.0	44.1	0.1	±0.8
39.0	39.4	0.4	±0.8

Function : 8. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
Fast	200	136.0	0.0	±0.5
	2	118.9	-0.1	+1.0 ; -1.5
	0.25	109.8	-0.2	+1.0 ; -3.0
Slow	200	129.5	-0.1	±0.5
	2	109.9	-0.1	+1.0 ; -3.0
	200	130.0	0.0	±0.5
LAE	2	110.1	0.1	+1.0 ; -1.5
	0.25	101.0	0.0	+1.0 ; -3.0

Function : 9. Peak C sound level

Number of cycles in test signal	Anticipated Value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
Complete cycle	135.4	134.8	-0.6	±2.0
Positive half cycle	134.4	134.0	-0.4	±1.0
Negative half cycle	134.4	134.0	-0.4	±1.0

เอกสารไม่ควบคุม

Page 5 of 6

F-CAL-005 Ed.1

Certificate No.: CP20240287EA

Calibration Report

Function : 5. Frequency and time weighting at 1 kHz

5.1 Frequency weighting at 1 kHz

Frequency Weighting	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
C-weighting	94.0	0.0	±0.2
A-weighting	94.0	0.0	±0.2
Z-weighting	94.0	0.0	±0.2

5.2 Time weighting at 1 kHz

Time Weighting	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
Fast	94.0	0.0	±0.1
Slow	94.0	0.0	±0.1
LAeq	94.0	0.0	±0.1

Function : 6. Long-Term Stability

Long-term stability over 30 minutes, with steady 1 kHz signal at reference level.

Time Period to Apply Signal (min)	Reference SPL (dB)	Record SPL at Conclusion of Time Period (dB)	Deviated value (dB)	Acceptance limits (dB)
30	94.0	94.0	0.0	±0.1

Function : 7. Level Linearity on the reference level range

7.1 Level Linearity on the reference level range, Upper

Anticipated Value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
94.0	94.0	0.0	±0.8
99.0	99.0	0.0	±0.8
104.0	104.0	0.0	±0.8
109.0	109.0	0.0	±0.8
114.0	114.0	0.0	±0.8
119.0	119.0	0.0	±0.8
124.0	124.0	0.0	±0.8
129.0	129.0	0.0	±0.8
134.0	134.0	0.0	±0.8
139.0	139.0	0.0	±0.8
140.0	140.0	0.0	±0.8

เอกสารไม่ควบคุม

Page 4 of 6

F-CAL-005 Ed.1

Certificate No.: CP20240287EA

Calibration Report

Function : 10. Overload indication

Measured value (dB)		Deviated value (dB)	Acceptance limits (dB)
Positive one-half cycle	Negative one-half cycle		
144.3	144.2	-0.1	±1.5

Function : 11. High-Level Stability

High-level stability over 5 minutes, with steady 1 kHz signal, 1 dB below upper boundary.

Time Period to Apply Signal (min)	Reference SPL (dB)	Record SPL at Conclusion of Time Period (dB)	Deviated value (dB)	Acceptance limits (dB)
5	139.0	139.0	0.0	±0.1

Uncertainty of measurement

Function	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1) Indication at the calibration check frequency	0.30	Not applicable
2) Self-generated Noise	0.10	Not applicable
3) Acoustical signal tests of frequency weightings - Free-field sound pressure response level	0.30	0.60 (10Hz to 4kHz) 0.70 (>4kHz to 10kHz)
4) Electrical signal tests of frequency weightings	0.20	0.20
5) Frequency and time weighting at 1 kHz	0.20	0.20
6) Long-Term Stability	0.10	0.10
7) Level Linearity on the reference level range	0.30	0.30
8) Tone burst response	0.20	0.30
9) Peak C sound level	0.20	0.35
10) Overload indication	0.20	0.25
11) High-Level Stability	0.10	0.10

Remarks:

1. Indication at the calibration check frequency can not measured because customer does not provide a sound calibrator.
2. The acceptance limit is for the deviated value.
3. Acceptance limits was IEC61672-3:2013 Class 1.
4. The coverage factor $k = 2.00$

- - End of Report - -

เอกสารไม่ควบคุม

Page 6 of 6

F-CAL-005 Ed.1



ELECTRICAL AND ELECTRONICS INSTITUTE FOUNDATION FOR INDUSTRIAL DEVELOPMENT

975 Moo 4, Bangpoo Industrial Estate, Soi 8, Sukhumvit Road km 37,
Phraek Sa, Mueang Samut Prakan, Samut Prakan 10280
Tel: +66 2709 4860 Fax: +66 2324 0917



Certificate No.: CP20240289EA
Operation No.: CP2024070252

Certificate of Calibration

Equipment: Sound Level Meter

Manufacturer: Larson Davis (Meter), PCB (Microphone), PCB (Preamplifier)

Model/Type: LxT1 (Meter), 377B02 (Microphone), PRMLxT1 (Preamplifier)

Serial No.: 0007310 (Meter), 345240 (Microphone), 077645 (Preamplifier)

ID No.: UAE.EFM.042/2566

Customer: United Analyst and Engineering Consultant Co.,Ltd.

Address: 81 Soi Udomsuk 41, Sukhumvit Road, Bangchak
Phrakhanong, Bangkok 10260

Received Date: 25 July 2024

Calibrated Date: 5 - 6 August 2024

Issued Date: 7 August 2024

Calibrated by: Ms. Juntaporn Kunhakom

Approved by:

(Mr. Sittichai Swaksuriyawong)
Group Manager

This report was prepared electronically using applicable electronic signature. Printing or copy of file are considered as a copy of the document.

The reported uncertainty of measurement was based on standard uncertainty multiplied by a coverage factor (k)
providing a level of confidence of approximately 95%. This certificate may not be reproduced other than in full except
with the prior written approval of the Electrical and Electronics Institute, Foundation for Industrial Development.

Page 1 of 6

เอกสารไม่ควบคุม

F-CAL-004 Ed.1



ELECTRICAL AND ELECTRONICS INSTITUTE FOUNDATION FOR INDUSTRIAL DEVELOPMENT

Certificate No.: CP20240289EA

Calibration Report

Equipment: Sound Level Meter

Manufacturer: Larson Davis (Meter), PCB (Microphone), PCB (Preamplifier)

Model/Type: LxT1 (Meter), 377B02 (Microphone), PRMLxT1 (Preamplifier)

Serial No.: 0007310 (Meter), 345240 (Microphone), 077645 (Preamplifier)

ID No.: UAE.EFM.042/2566

Ambient Temperature: (23 ± 2) °C

Relative Humidity: (50 ± 15) %

Pressure: (101.3 ± 1.5) kPa

Method of Calibration :-
IEC 61672-3:2013.

Condition of this result of calibration

1. Reference standards instrument :-

Instrument	Model	Serial No.	Cert. No.	Due Date
1) Standard microphone	4180	2787490	AA-1012-23	12 November 2024
2) Arbitrary Function Generator	AFG2021	C010063	CK20240048EA	23 June 2025
3) Programmable Attenuator	PA5	2755	EF-0040-23	1 October 2024
4) 6.5 Digit precision multimeter	8846A	9610014	CB20230200EA	15 November 2024
5) Pressure humidity and Temperature Transmitter	PTU301	L3950483	CL1-P240023 CD20240142EA	24 March 2025 12 June 2025
6) Pressure humidity and Temperature Transmitter	PTU301	L3950484	CL1-P240030 CD20240143EA	11 April 2025 12 June 2025
7) Performance Audio Analyzer	U8903B	MY56510003	CB20240035EB CK20230072EA	13 February 2025 13 September 2024

2. This result of calibration was found accurate as shown on date and place of calibration only.

3. This certification is traceable to the international system of unit maintained at :-

Reference standards instrument for Acoustic function

- National Institute of Metrology (Thailand)

Reference standards instrument for Electrical function

- National Institute of Metrology (Thailand)

- Electrical and Electronics Institute; NSC Accredited Calibration No.0119

Result of Calibration:-

Function : 1. Indication at the calibration check frequency

Reference Acoustic Signal (dB)	Measured value (dB)	Deviation (dB)	Acceptance limits (dB)
-	-	-	-

Page 2 of 6

F-CAL-005 Ed.1

เอกสารไม่ควบคุม



ELECTRICAL AND ELECTRONICS INSTITUTE FOUNDATION FOR INDUSTRIAL DEVELOPMENT

Certificate No.: CP20240289EA

Calibration Report

Function : 2. Self-generated Noise

2.1 Microphone Installed

Measured value (dB)
30.3

2.2 Microphone replaced by the electrical input signal device

Frequency Weighting	Measured value (dB)
A-weighting	30.1
C-weighting	30.0
Z-weighting	35.7

Function : 3. Acoustical signal tests of frequency weightings (Without Windscreen)

Meter free-field acoustic response at a level of 84 dB.

Frequency (Hz)	Deviation from various Frequency Weighting Response Curve			
	C-Weighting (dB)	A-Weighting (dB)	Z-Weighting (dB)	Acceptance limits (dB)
125	0.3	0.2	0.3	±1.0
1000	0.2	0.2	0.2	±0.7
8000	-0.2	-0.1	-0.1	+1.5; -2.5

Function : 4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various Frequency Weighting Response Curve			
	C-Weighting (dB)	A-Weighting (dB)	Z-Weighting (dB)	Acceptance limits (dB)
63	-0.1	0.1	0.0	±1.0
125	0.0	0.0	0.0	±1.0
250	0.0	0.0	0.0	±1.0
500	0.0	0.0	0.0	±1.0
1000	0.0	0.0	0.0	±0.7
2000	0.0	0.1	0.0	±1.0
4000	0.0	0.0	0.0	±1.0
8000	-0.1	0.0	0.0	+1.5; -2.5
16000	0.0	0.0	-0.1	+2.5; -16.0

เอกสารไม่ควบคุม

Page 3 of 6

F-CAL-005 Ed.1



ELECTRICAL AND ELECTRONICS INSTITUTE FOUNDATION FOR INDUSTRIAL DEVELOPMENT

Certificate No.: CP20240289EA

Calibration Report

Function : 5. Frequency and time weighting at 1 kHz

5.1 Frequency weighting at 1 kHz

Frequency Weighting	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
C-weighting	94.0	0.0	±0.2
A-weighting	94.0	0.0	±0.2
Z-weighting	94.0	0.0	±0.2

5.2 Time weighting at 1 kHz

Time Weighting	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
Fast	94.0	0.0	±0.1
Slow	94.0	0.0	±0.1
LAeq	94.0	0.0	±0.1

Function : 6. Long-Term Stability

Long-term stability over 30 minutes, with steady 1 kHz signal at reference level.

Time Period to Apply Signal (min)	Reference SPL (dB)	Record SPL at Conclusion of Time Period (dB)	Deviated value (dB)	Acceptance limits (dB)
30	94.0	94.0	0.0	±0.1

Function : 7. Level Linearity on the reference level range

7.1 Level Linearity on the reference level range, Upper

Anticipated Value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
94.0	94.0	0.0	±0.8
99.0	99.0	0.0	±0.8
104.0	104.0	0.0	±0.8
109.0	109.0	0.0	±0.8
114.0	114.0	0.0	±0.8
119.0	119.0	0.0	±0.8
124.0	124.0	0.0	±0.8
129.0	129.0	0.0	±0.8
134.0	134.0	0.0	±0.8
139.0	139.0	0.0	±0.8
140.0	140.0	0.0	±0.8
141.0	141.0	0.0	±0.8

เอกสารไม่ควบคุม

Page 4 of 6

F-CAL-005 Ed.1

Certificate No.: CP20240289EA

Calibration Report

7.2 Level Linearity on the reference level range, Lower

Anticipated Value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
94.0	94.0	0.0	±0.8
89.0	89.0	0.0	±0.8
84.0	84.0	0.0	±0.8
79.0	79.0	0.0	±0.8
74.0	74.0	0.0	±0.8
69.0	69.0	0.0	±0.8
64.0	64.0	0.0	±0.8
59.0	59.0	0.0	±0.8
54.0	54.0	0.0	±0.8
49.0	49.0	0.0	±0.8
44.0	44.1	0.1	±0.8
39.0	39.4	0.4	±0.8

Function : 8. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
Fast	200	135.9	-0.1	±0.5
	2	118.8	-0.2	+1.0 ; -1.5
	0.25	109.8	-0.2	+1.0 ; -3.0
Slow	200	129.5	-0.1	±0.5
	2	109.9	-0.1	+1.0 ; -3.0
	200	130.0	0.0	±0.5
LAE	2	110.0	0.0	+1.0 ; -1.5
	0.25	100.9	-0.1	+1.0 ; -3.0

Function : 9. Peak C sound level

Number of cycles in test signal	Anticipated Value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
Complete cycle	135.4	134.8	-0.6	±2.0
Positive half cycle	134.4	134.0	-0.4	±1.0
Negative half cycle	134.4	134.0	-0.4	±1.0

Page 5 of 6

F-CAL-005 Ed.1

เอกสารไม่ควบคุม

Certificate No.: CP20240289EA

Calibration Report

Function : 10. Overload indication

Measured value (dB)		Deviated value (dB)	Acceptance limits (dB)
Positive one-half cycle	Negative one-half cycle		
144.3	144.2	-0.1	±1.5

Function : 11. High-Level Stability

High-level stability over 5 minutes, with steady 1 kHz signal, 1 dB below upper boundary.

Time Period to Apply Signal (min)	Reference SPL (dB)	Record SPL at Conclusion of Time Period (dB)	Deviated value (dB)	Acceptance limits (dB)
5	139.0	139.0	0.0	±0.1

Uncertainty of measurement

Function	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1) Indication at the calibration check frequency	0.30	Not applicable
2) Self-generated Noise	0.10	Not applicable
3) Acoustical signal tests of frequency weightings - Free-field sound pressure response level	0.30	0.60 (10Hz to 4kHz) 0.70 (>4kHz to 10kHz)
4) Electrical signal tests of frequency weightings	0.20	0.20
5) Frequency and time weighting at 1 kHz	0.20	0.20
6) Long-Term Stability	0.10	0.10
7) Level Linearity on the reference level range	0.30	0.30
8) Tone burst response	0.20	0.30
9) Peak C sound level	0.20	0.35
10) Overload indication	0.20	0.25
11) High-Level Stability	0.10	0.10

Remarks:

1. Indication at the calibration check frequency can not measured because customer does not provide a sound calibrator.
2. The acceptance limit is for the deviated value.
3. Acceptance limits was IEC61672-3:2013 Class 1.
4. The coverage factor $k = 2.00$

- - End of Report - -

Page 6 of 6

F-CAL-005 Ed.1

เอกสารไม่ควบคุม

Certificate No.: CP20240288EA

Operation No.: CP2024070251

Certificate of Calibration

Equipment: Sound Level Meter

Manufacturer: Larson Davis (Meter), PCB (Microphone), PCB (Preamplifier)

Model/Type: LxT1 (Meter), 377B02 (Microphone), PRMLxT1 (Preamplifier)

Serial No.: 0007312 (Meter), 345818 (Microphone), 077647 (Preamplifier)

ID No.: UAE.EFM.044/2566

Customer: United Analyst and Engineering Consultant Co.,Ltd.

Address: 81 Soi Udomsuk 41, Sukhumvit Road, Bangchak Phrakhanong, Bangkok 10260

Received Date: 25 July 2024

Calibrated Date: 5 - 6 August 2024

Issued Date: 7 August 2024

Calibrated by: Ms. Juntaporn Kunhakom

Approved by:

(Mr. Sittichai Swaksuriyawong)
Group Manager

This report was prepared electronically using applicable electronic signature. Printing or copy of file are considered as a copy of the document.

The reported uncertainty of measurement was based on standard uncertainty multiplied by a coverage factor (k) providing a level of confidence of approximately 95%. This certificate may not be reproduced other than in full except with the prior written approval of the Electrical and Electronics Institute, Foundation for Industrial Development.

Page 1 of 6

เอกสารไม่ควบคุม

F-CAL-004 Ed.1

Certificate No.: CP20240288EA

Calibration Report

Equipment: Sound Level Meter

Manufacturer: Larson Davis (Meter), PCB (Microphone), PCB (Preamplifier)

Model/Type: LxT1 (Meter), 377B02 (Microphone), PRMLxT1 (Preamplifier)

Serial No.: 0007312 (Meter), 345818 (Microphone), 077647 (Preamplifier)

ID No.: UAE.EFM.044/2566

Ambient Temperature: (23 ± 2) °C

Relative Humidity: (50 ± 15) %

Pressure: (101.3 ± 1.5) kPa

Method of Calibration :- IEC 61672-3:2013.

Condition of this result of calibration

1. Reference standards instrument :-

Instrument	Model	Serial No.	Cert. No.	Due Date
1) Standard microphone	4180	2787490	AA-1012-23	12 November 2024
2) Arbitrary Function Generator	AFG2021	C010063	CK20240048EA	23 June 2025
3) Programmable Attenuator	PA5	2755	EF-0040-23	1 October 2024
4) 6.5 Digit precision multimeter	8846A	9610014	CB20230200EA	15 November 2024
5) Pressure humidity and Temperature Transmitter	PTU301	L3950483	CL1-P240023 CD20240142EA	24 March 2025 12 June 2025
6) Pressure humidity and Temperature Transmitter	PTU301	L3950484	CL1-P240030 CD20240143EA	11 April 2025 12 June 2025
7) Performance Audio Analyzer	U8903B	MY56510003	CB20240035EB CK20230072EA	13 February 2025 13 September 2024

2. This result of calibration was found accurate as shown on date and place of calibration only.

3. This certification is traceable to the international system of unit maintained at :-

Reference standards instrument for Acoustic function

- National Institute of Metrology (Thailand)

Reference standards instrument for Electrical function

- National Institute of Metrology (Thailand)
- Electrical and Electronics Institute; NSC Accredited Calibration No.0119

Result of Calibration:-

Function : 1. Indication at the calibration check frequency

Reference Acoustic Signal (dB)	Measured value (dB)	Deviation (dB)	Acceptance limits (dB)
-	-	-	-

Page 2 of 6

F-CAL-005 Ed.1

เอกสารไม่ควบคุม

Certificate No.: CP20240288EA

Calibration Report

Function : 2. Self-generated Noise

2.1 Microphone Installed

Measured value (dB)
28.5

2.2 Microphone replaced by the electrical input signal device

Frequency Weighting	Measured value (dB)
A-weighting	28.4
C-weighting	28.3
Z-weighting	34.1

Function : 3. Acoustical signal tests of frequency weightings (Without Windscreen)

Meter free-field acoustic response at a level of 84 dB.

Frequency (Hz)	Deviation from various Frequency Weighting Response Curve			
	C-Weighting (dB)	A-Weighting (dB)	Z-Weighting (dB)	Acceptance limits (dB)
125	0.2	0.1	0.1	±1.0
1000	0.0	0.0	0.0	±0.7
8000	-0.9	-0.9	-0.8	+1.5; -2.5

Function : 4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various Frequency Weighting Response Curve			
	C-Weighting (dB)	A-Weighting (dB)	Z-Weighting (dB)	Acceptance limits (dB)
63	0.0	0.1	0.0	±1.0
125	0.0	0.0	0.0	±1.0
250	0.0	0.0	0.0	±1.0
500	0.0	-0.1	0.0	±1.0
1000	0.0	0.0	0.0	±0.7
2000	0.0	0.0	0.0	±1.0
4000	0.0	0.0	0.0	±1.0
8000	-0.1	0.0	0.0	+1.5; -2.5
16000	0.0	0.0	-0.1	+2.5; -16.0

เอกสารไม่ควบคุม

Page 3 of 6

F-CAL-005 Ed.1

Certificate No.: CP20240288EA

Calibration Report

Function : 5. Frequency and time weighting at 1 kHz

5.1 Frequency weighting at 1 kHz

Frequency Weighting	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
C-weighting	94.0	0.0	±0.2
A-weighting	94.0	0.0	±0.2
Z-weighting	94.0	0.0	±0.2

5.2 Time weighting at 1 kHz

Time Weighting	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
Fast	94.0	0.0	±0.1
Slow	94.0	0.0	±0.1
LAeq	94.0	0.0	±0.1

Function : 6. Long-Term Stability

Long-term stability over 30 minutes, with steady 1 kHz signal at reference level.

Time Period to Apply Signal (min)	Reference SPL (dB)	Record SPL at Conclusion of Time Period (dB)	Deviated value (dB)	Acceptance limits (dB)
30	94.0	94.0	0.0	±0.1

Function : 7. Level Linearity on the reference level range

7.1 Level Linearity on the reference level range, Upper

Anticipated Value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
94.0	94.0	0.0	±0.8
99.0	99.0	0.0	±0.8
104.0	104.0	0.0	±0.8
109.0	109.0	0.0	±0.8
114.0	114.0	0.0	±0.8
119.0	119.0	0.0	±0.8
124.0	124.0	0.0	±0.8
129.0	129.0	0.0	±0.8
134.0	134.0	0.0	±0.8
139.0	139.0	0.0	±0.8

เอกสารไม่ควบคุม

Page 4 of 6

F-CAL-005 Ed.1

Certificate No.: CP20240288EA

Calibration Report

7.2 Level Linearity on the reference level range, Lower

Anticipated Value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
94.0	94.0	0.0	±0.8
89.0	89.0	0.0	±0.8
84.0	84.0	0.0	±0.8
79.0	79.0	0.0	±0.8
74.0	74.0	0.0	±0.8
69.0	69.0	0.0	±0.8
64.0	64.0	0.0	±0.8
59.0	59.0	0.0	±0.8
54.0	54.0	0.0	±0.8
49.0	49.0	0.0	±0.8
44.0	44.1	0.1	±0.8
39.0	39.3	0.3	±0.8

Function : 8. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
Fast	200	136.0	0.0	±0.5
	2	118.8	-0.2	+1.0; -1.5
	0.25	109.7	-0.3	+1.0; -3.0
Slow	200	129.5	-0.1	±0.5
	2	109.9	-0.1	+1.0; -3.0
	200	130.0	0.0	±0.5
LAE	2	110.0	0.0	+1.0; -1.5
	0.25	100.9	-0.1	+1.0; -3.0

Function : 9. Peak C sound level

Number of cycles in test signal	Anticipated Value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
Complete cycle	135.4	134.8	-0.6	±2.0
Positive half cycle	134.4	134.0	-0.4	±1.0
Negative half cycle	134.4	134.0	-0.4	±1.0

เอกสารไม่ควบคุม

Page 5 of 6

F-CAL-005 Ed.1

Certificate No.: CP20240288EA

Calibration Report

Function : 10. Overload indication

Measured value (dB)		Deviated value (dB)	Acceptance limits (dB)
Positive one-half cycle	Negative one-half cycle		
142.4	142.3	-0.1	±1.5

Function : 11. High-Level Stability

High-level stability over 5 minutes, with steady 1 kHz signal, 1 dB below upper boundary.

Time Period to Apply Signal (min)	Reference SPL (dB)	Record SPL at Conclusion of Time Period (dB)	Deviated value (dB)	Acceptance limits (dB)
5	139.0	139.0	0.0	±0.1

Uncertainty of measurement

Function	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1) Indication at the calibration check frequency	0.30	Not applicable
2) Self-generated Noise	0.10	Not applicable
3) Acoustical signal tests of frequency weightings - Free-field sound pressure response level	0.30	0.60 (10Hz to 4kHz) 0.70 (>4kHz to 10kHz)
4) Electrical signal tests of frequency weightings	0.20	0.20
5) Frequency and time weighting at 1 kHz	0.20	0.20
6) Long-Term Stability	0.10	0.10
7) Level Linearity on the reference level range	0.30	0.30
8) Tone burst response	0.20	0.30
9) Peak C sound level	0.20	0.35
10) Overload indication	0.20	0.25
11) High-Level Stability	0.10	0.10

Remarks:

1. Indication at the calibration check frequency can not measured because customer does not provide a sound calibrator.
2. The acceptance limit is for the deviated value.
3. Acceptance limits was IEC61672-3:2013 Class 1.
4. The coverage factor $k = 2.00$

- - End of Report - -

เอกสารไม่ควบคุม

Page 6 of 6

F-CAL-005 Ed.1



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000-29 FAX. 0-2719-9484



Cert.No.: 24CH311
Page.: 1 of 3

Certificate of Calibration

Equipment : pH Meter
Manufacturer : EcoSense
Model : pH100A
Serial No. : JC04740
ID No. : UAE.EFM.062/2566(EFM,pH.05/66)
Condition As-Received: Used Item
Received Date : 12 March 2024
Calibration Date : 13 March 2024
Reference : 2403-0386WSC-4
Submitted by : United Analyst and Engineering Consultant Co.,Ltd.
3 Soi Udomsuk 41, Sukhumvit Road,
Bangchak, Phrakhanong, Bangkok 10260
Ambient Temperature : (25 ± 2.5) °C
Relative Humidity : (50 ± 15) %
Calibration Procedure : In - house method :
- CP-CH5 by direct measurement with DC voltage
standard and direct measurement with
certified reference material (CRM)
- CP-CH8 by comparison with temperature standard

Calibrated by : Warakorn Lernagatrakul

Approved by :

Saithip
Approved Signatory

() Pornthippa Tameyakul
() Unnopphol Harachai
(✓) Saithip Meangmai

Issue Date : 15 March 2024

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3: Equipment Calibration and Testing Services

เอกสารไม่ควบคุม

A 0064528



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000 FAX. 0-2719-9484

Cert.No.: 24CH311
Page.: 2 of 3

Condition of this calibration result

1. Reference Standard Instrument

Instrument	Serial No.	ID No.	Cert. No.	Due Date
1) Document Process Calibrator	54030049	130RC116	23E2802	27 Aug 2024
2) Ref. Standard Thermometer	4982054	110RC044	23I908	26 July 2024

This certification is traceable to the International System of Unit maintained through:-
- Technology Promotion Association (Thailand-Japan)

2. Certified Reference Materials : The measurement results are traceable to SI through CPA chem Ltd.,
ANSI-ASQ National Accreditation Board, Accredited No. AR-1835

Buffer Solution	Manufacturer	Lot No.	Exp. date
pH 4.008	CPA chem	940102	27 Nov 2025
pH 6.986	CPA chem	940104	02 Nov 2024
pH 9.997	CPA chem	940106	02 Nov 2024

3. This certificate is valid only to the item calibrated on date and place of calibration.

Calibration Results

Function : mV Measurement

Performing standard curve by Document Process Calibrator at pH (4,7)(7,10)

Unit Under Calibration	Nominal Value	Standard Voltage Input	Actual Reading		Uncertainty of Measurement	Coverage factor
	pH	mV	mV	pH	(±mV)	k
pH Meter S/N: JC04740	4.00	177.48	177	4.01	0.58	2.00
	7.00	0.00	0	7.00	0.58	2.00
	7.00	0.00	0	7.00	0.58	2.00
	10.00	-177.48	-177	10.01	0.58	2.00

เอกสารไม่ควบคุม

a 1206339



Cert.No.: 24CH311
Page.: 3 of 3

Calibration Results

Function : pH Measurement

Performing three buffers standard curve by using buffer nominal pH (4,7)(7,10)

Unit Under Calibration	Standard pH Buffer Solution	Actual pH Reading	Actual mV Reading (mV)	Uncertainty of pH Measurement (±)	Coverage factor k
pH Electrode S/N : 230906SIA605377	4.008	4.01	172	0.0071	2.00
	6.986	7.00	-2	0.0099	2.00
	6.986	7.00	-2	0.011	2.00
	9.997	10.01	-177	0.0096	2.00

Function : Temperature Measurement

(*) Without adjustment

This equipment was connected with Temperature Probe;

- Model :
- Serial No. : 230906SIA605377
Dimension of probe
- Length : 110 mm.
- Diameter : 12 mm.
- Immersion Depth : 100 mm.

Calibration Point (°C)	Standard Temperature (°C)	UUC* Reading (°C)	Error (°C)	Uncertainty of measurement (± °C)	Coverage factor k
25.0	25.004	24.9	-0.104	0.13	2.00
30.0	30.002	29.9	-0.102	0.13	2.00
35.0	35.002	34.9	-0.102	0.13	2.00

Remark : - UUC* = Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k, providing a level of confidence of approximately 95 %.

-000-

เอกสารไม่ควบคุม

a 1206340



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000 FAX. 0-2719-9484

Cert.No.: 24TW56
Page.: 1 of 2

Certificate of Testing

Equipment : DO Meter
Manufacturer : Horiba
Model : LAQUA-DO210
Serial No. : HE2L0031
ID No. : UAE.EFM.020/2566(EFM.DO.05/66)
Received Date : 12 March 2024
Test Date : 13 March 2024
Reference : 2403-0385WSC-1
Submitted by : United Analyst and Engineering Consultant Co.,Ltd.
3 Soi Udomsuk 41, Sukhumvit Road, Bangchak,
Phrakhanong, Bangkok 10260
Laboratory Condition : Temperature (25 ± 5) °C
Humidity (50 ± 20) %
Test Procedure : In - house method : CP-CH9
by Comparison Technique with Azide Modification Method
Tested by : Walalak Sirithean
Approved by : *Saithip*
Approved Signatory
() Pornthippa Tameyakul
() Unnopphol Harachai
(✓) Saithip Meangmai

Issue Date : 15 March 2024

เอกสารไม่ควบคุม



Cert.No.: 24TW56
Page: 2 of 2

Condition of this result of calibration

1. Reference Standard Instruments :

This certification is traceable to the International System of Unit through the reference standards laboratory of Industrial Calibration Center, Technology Promotion Association (Thailand-Japan).

Instruments	Serial No.	ID No.	Certificate No.	Due Date
1. Burette	-	130BU10	23CG1172	22 Mar 2025
2. Balance	14233821	110RC001	23MM405	16 July 2024

2. Standard Material :-

Material	Manufacturer	Lot.No.	Assay
Sodium Thiosulfate pentahydrate	Merck	AM1763316	100.2%

Result : Dissolved Oxygen Meter Adjustment With Air 100 %
Dissolved Oxygen Probe No.: 9K2H0053

Titration Method (Azide Modification Method) (mg/L)	DO Meter Reading (mg/L)	Standard Deviation (mg/L)
8.18	8.19	0.0055

This report was certified only for the instrument we tested. It is allowable to use for study
Intend to use for advertising and referral purpose is prohibited. This report may not be reproduced
other in full without written approval of the laboratory

-000-

เอกสารไม่ควบคุม



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL: 0-2717-3000-29 FAX: 0-2719-9484



Cert. No.: 24LM41
Page: 1 of 2

Certificate of Calibration

Equipment : DO Meter With Sensor
Manufacturer : Horiba
Model : LAQUA-DO210
Serial No. : HE2L0031
ID No. : UAE.EFM.020/2566(EFM.DO.05/66)
Submitted by : United Analyst and Engineering Consultant Co.,Ltd.
3 Soi Udomsuk 41, Sukhumvit Road,
Bangchak, Phrakhanong,
Bangkok 10260
Location : TPA Chemistry Calibration Laboratory
Received Order : 12 March 2024
Calibrated Date : 14 March 2024
Ambient Temperature : (26 ± 10) °C
Relative Humidity : (50 ± 30) %
AC Line Voltage : (220 ± 22) V
Calibrated by : Preecha Hiahib
Approved by :
() Pornthippa Tameyakul
() Unnopphol Harachai
(✓) Suwit Imjai
Issue Date : 29 March 2024

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3: Equipment Calibration and Testing Services.

เอกสารไม่ควบคุม



Equipment : DO Meter With Sensor
Condition As-Received : Used Item
Reference : 2403-0385WSC-2
Procedure Used :-
Calibration were conducted using in-house calibration procedure CP-OT01 according to comparison with
Industrial Platinum Resistance Thermometer (IPRT) into Temperature Bath.
The temperature scale used was based on ITS-90.

Cert. No.: 24LM41
Page: 2 of 2

Condition of this result of calibration

1. Reference standard instrument :-

Instrument	Serial No.	Cert. No.	Traceable	Due Date
1) Digital Thermometer	A52847	2311222	TPA	10 Oct 2024

2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certification is traceable to the International System of Unit.

Remark : TPA : Technology Promotion Association (Thailand - Japan)

Result of Calibration :- (*) Without Adjustment

Function : Temperature measurement.

This instrument was connected with temperature sensor, S/N: 9K2H0053

Calibration Point (°C)	Immersion Depth (mm)	Standard Temperature (°C)	UUC* Reading (°C)	Error (°C)	Uncertainty (± °C)	Coverage Factor k
25.0	100	25.005	25.1	0.095	0.16	2.00
30.0	100	30.004	30.0	-0.004	0.16	2.00
35.0	100	35.002	35.0	-0.002	0.16	2.00

UUC* : Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a
coverage factor *k*, providing a level of confidence of approximately 95 %

-000-

เอกสารไม่ควบคุม



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL: 0-2717-3000-29 FAX: 0-2719-9484



Cert.No.: 24CH322
Page: 1 of 3

Certificate of Calibration

Equipment : Conductivity Meter
Manufacturer : Horiba
Model : LAQUA-EC210
Serial No. : HC9L0015
ID No. : UAE.EFM.010/2563(EFM.SCT.04/63)
Condition As-Received: Used Item
Received Date : 12 March 2024
Calibration Date : 14 March 2024
Reference : 2403-0387WSC-2
Submitted by : United Analyst and Engineering Consultant Co.,Ltd.
3 Soi Udomsuk 41, Sukhumvit Road,
Bangchak, Phrakhanong, Bangkok 10260
Ambient Temperature : (25 ± 2.5) °C
Relative Humidity : (50 ± 15) %
Calibration Procedure:
In-house method :
- CP-CH6 by direct measurement with
certified reference material (CRM)
- CP-CH8 by Comparison with temperature standard
Calibrated by : Warakorn Lemgatrakul
Approved by :
() Pornthippa Tameyakul
() Unnopphol Harachai
(✓) Saithip Meangmai
Issue Date : 15 March 2024

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3: Equipment Calibration and Testing Services.

เอกสารไม่ควบคุม

A 0064532



Cert.No.: 24CH322

Page.: 2 of 3

Condition of this result of calibration

1. Reference Standard Instrument :-

Instrument	Serial No.	ID No.	Certificate No.	Due date
1) Thermometer	1963878	130RC095	231051	05 Sep 2024
2) Ref. Std. Thermometer	4952054	110RC044	231908	26 July 2024

- This Certification is traceable to SI Through Technology Promotion Association (Thailand - Japan)

2. Certified Reference Materials :-

- Conductivity calibration solution, CPA chem Ltd., The measurement results are traceable to SI through CPA chem Ltd., ANSI-ASQ National Accreditation Board, Accredited No. AR-1835

Conductivity Solution	Manufacturer	Lot No.	Exp. date
1413.0 µS/cm	CPA Chem	936624	19 Oct 2024
12.880 mS/cm	CPA Chem	931956	30 Sep 2024

- Control Conductivity calibration solution temperature by Water bath (25 ± 0.1) °C

3. This certificate is valid only to the item calibrated on date and place of calibration.

Calibration results**Function : Conductivity Measurement**

(*) After Adjustment at 1413.0 µS/cm

Conductivity Electrode Serial No.: 9B9F0277

Standard Conductivity Solution	Before Adjustment UUC* Reading	After Adjustment UUC* Reading	Uncertainty of Measurement (±)	Coverage factor k
1413.0 µS/cm	1436 µS/cm	1413 µS/cm	9.2 µS/cm	2.00
12.880 mS/cm	13.22 mS/cm	12.95 mS/cm	0.086 mS/cm	2.00

Remark : - UUC* = Unit Under Calibration

เอกสารไม่ควบคุม

a 1206347



Cert.No.: 24CH322

Page.: 3 of 3

Calibration Results**Function : Temperature Measurement**

This equipment was connected with Temperature Probe;

- Model :	9383
- Serial No. :	9B9F0277

Dimension of probe;

- Length :	110 mm
- Diameter :	10 mm
- Immersion Depth :	90 mm

Calibration Result : Without adjustment

Calibration Point (°C)	Standard Temperature (°C)	UUC* Reading (°C)	Error (°C)	Uncertainty of Measurement (± °C)	Coverage factor k
25.0	25.003	25.0	-0.003	0.13	2.00
30.0	30.002	30.0	-0.002	0.13	2.00
35.0	35.003	35.0	-0.003	0.13	2.00

Remark : - UUC* = Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k, providing a level of confidence of approximately 95 %.

-o-o-

เอกสารไม่ควบคุม

a 1206348

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7-139 MOO 13, SOI SINTINAKORN 11 TAMBON BANG KHAO,
AMPHOE BANG PHU, SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL: 0809-2116-5800-1 FAX: 0809-2116-7140



Page 3/7

Certificate of Calibration**Customer**

Name : UNITED ANALYST AND ENGINEERING CONSULTANT CO., LTD.
Address : XI Soi Udomsak 41, Sukhumvit Road, Bangchak, Prakanong,
Bangkok 10260

Certificate No : 24-AFM-101

Request No : Req-2024-1062

Unit Under Calibration Details

Measurement Item : Air Flow Meter
Manufacturer : TSI
Model : 4146 Sensor Model : -
Serial Number : 41462317033 Sensor Serial Number : -
ID : UAE EFM 080/2566

Location of Calibration : LAB 4 AIR VELOCITY METER

Calibration Environment and Details

Temperature : 23 °C ± 3 °C
Humidity : 55 %RH ± 20 %RH
Barometric Pressure : 1013 hPa ± 10 hPa
Received Date : 13 May 2024
Calibration Date : 24 May 2024
Calibration Procedure : In-house method CP-AFM-01 by Comparison technique with Standard Primary Flow Calibrator

Reference Standard	Model	Serial Number	Traceable	Due Calibration
Air Flow Meter	Gilibrator 3 Low flow	18501010006	Sensidyne	12 July 2024
Air Flow Meter	Gilibrator 3 Standard flow	19031011005	Sensidyne	12 July 2024
Temperature meter	GT 11	08000057	Oreborn	1 March 2025
Pressure meter	CPG2400	41000KDU/651882	TPA	9 November 2024

Traceability :

This Certificate is traceable to SI Unit through Sensidyne A2LA Accreditation No. 3943.01

Note :

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor k = 2, providing a level of confidence approximately 95 %.

Calibration By :
Mr. Noppadon Luangrat
Service Calibration Engineer

Approved By :
Mr. Pacit Muthavorn
Calibration Engineer Supervisor
Issue Date : 24 May 2024

เอกสารไม่ควบคุม

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

FM-708-AFM-01 Rev.00 Issue date 01/07/19

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7-139 MOO 13, SOI SINTINAKORN 11 TAMBON BANG KHAO,
AMPHOE BANG PHU, SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL: 0809-2116-5800-1 FAX: 0809-2116-7140



Page 2/2

Certificate No : 24-AFM-101

Request No : Req-2024-1062

Result of Calibration :

Temperature (°C)	Pressure (kPa)	STD (l/min)	UUC (l/min)	Error (l/min)	Uncertainty (l/min)
23.00	100.65	0.020	0.020	0.000	0.0013
23.10	100.69	0.050	0.050	0.000	0.0033
23.00	100.68	0.100	0.100	0.000	0.0028
23.10	100.65	0.201	0.200	-0.001	0.0056
23.00	100.64	0.502	0.500	-0.002	0.0073
23.30	100.62	1.008	1.021	0.013	0.014
23.50	100.68	1.681	1.700	0.019	0.024
23.70	100.69	1.989	2.014	0.025	0.029
23.90	100.72	2.948	3.000	0.052	0.042
24.20	100.86	3.930	4.000	0.070	0.056
24.30	100.99	4.917	5.000	0.083	0.070

Note

STD : Standard

UUC : Unit Under Calibration

- UUC Reference Condition : At 21.1 °C, 101.3 kPa, Air

- Flow Rate was corrected for non-standard operating condition by using equation :

$$Q_{meas} = Q_{ref} \times \frac{P_{ref}}{P} \times \frac{T_{meas}}{T_{ref}}$$

where Q = Flow Rate

P = Absolute Pressure

T = Absolute Temperature

Meas = Measurement Condition

ref = Standard Condition

* Indicates non accredited

End of Certificate

เอกสารไม่ควบคุม

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

FM-708-AFM-01 Rev.00 Issue date 01/07/19



Certificate of Calibration

Certificate No. : 24P1145
Page : 1 of 2

Equipment : Aneroid Barometer

Manufacturer: Barigo

Model : 111MS

Serial No.: -

ID No.: UAE.EMA2.067/2552

Condition As-Received: Used Item

Received Date: 03 April 2024

Calibration Date: 09 April 2024

Reference: 2404-0119WSC

Submitted by: United Analyst and Engineering Consultant Co., Ltd.

Ambient Temperature: (23 ± 2) °C

Relative Humidity: (50 ± 15) %

Atmospheric Pressure: 1007 mbar

This certificate may not be reproduced other than in full,
except with the prior written approval of the head of
Corporate Services 3: Equipment Calibration and Testing Services.

81 Soi Udomsuk 41, Sukhumvit Road, Bangchak,
Phrakhanong, Bangkok 10260

Procedure used: The calibration was conducted by direct comparison method against Pressure Measuring Instruments
Standard according to calibration procedure CP-P10, using " DKD-R 6-1 ; Calibration of Pressure Gauges " as
a guidelines.

Condition of this result of calibration

1. Reference standards instruments :

Instrument	Model	Serial No.	Certificate No.	Due Date
1) Standard Barometer	DPI142	1422505046	MP-0094-23	03 May 2024

2. This instrument was installed in vertical orientation and center of the dial was used as the reference level.

3. This result of calibration was made on requested at the point specified by customer.

4. Scale and conversion factor is 1 kPa = 7.50062 mmHg

5. This result of calibration instrument was in absolute pressure.

6. This instrument was used clean air as pressure media.

7. The certificate is valid only to the item calibrated on date and place of calibration.

8. This Certification is traceable to the International System of Unit maintained through:-

- National Institute of Metrology Thailand (NIMT)

Calibrated by : Suksan Khankaew

Issue Date : 10 April 2024

Approved Signatory :

[] Phalinee Prabpaipal

[] Sura Suwannasri

[✓] Attapol Panurach

เอกสารไม่ควบคุม



Result of calibration:- Without adjustment

Function:- Absolute Pressure Measurement

Range : 720 mmHg to 780 mmHg

Scale Interval : 1 mmHg (The Fifth Estimate)

Increasing Pressure

Applied Pressure (mmHg)	717.86	729.00	739.73	750.27	761.74	773.61	786.17
UUC* Indication (mmHg)	720.0	730.0	740.0	750.0	760.0	770.0	780.0
Error (mmHg)	2.14	1.00	0.27	-0.27	-1.74	-3.61	-6.17

Decreasing Pressure

Applied Pressure (mmHg)	786.17	773.15	760.92	749.39	738.50	727.65	717.77
UUC* Indication (mmHg)	780.0	770.0	760.0	750.0	740.0	730.0	720.0
Error (mmHg)	-6.17	-3.15	-0.92	0.61	1.50	2.35	2.23

The uncertainty of measurement was ± 0.24 mmHg

* UUC = Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied
by a coverage factor $k = 2$, providing a level of confidence of approximately 95 %.

-000-

เอกสารไม่ควบคุม



Certificate of Calibration

Certificate No. : 24H716
Page : 1 of 2

Equipment : Digital Thermo-Hygrometer

Manufacturer: Digicon

Model : TH-02

Serial No.: 995034173

ID No.: UAE.EFM.162/2565

Condition As-Received: Used Item

Received Date: 06 April 2024

Calibration Date: 10 April 2024
to 11 April 2024

Reference: 2404-0245WSC

Submitted by: United Analyst and Engineering Consultant Co., Ltd.

Ambient Temperature: (26 ± 3) °C

Relative Humidity: (50 ± 20) %

81 Soi Udomsuk 41, Sukhumvit Road,
Bangchak, Phrakhanong, Bangkok 10260

Procedure used: Calibration were conducted using in-house calibration procedure CP-H03 according to comparison
with standard chilled mirror sensor for humidity measurement function and comparison with standard
temperature probe for temperature measurement function into humidity / temperature chamber.

Condition of this result of calibration

1. Reference standards instruments :

Instrument	Model	Serial No.	Certificate No.	Due Date
1) Chilled Mirror Hygrometer	Dew Master	44730	2165e	02 Aug 2024
2) Handheld Thermometer With Sensor	1521	ASA339	23H1238	16 Oct 2024

2. The certificate is valid only to the item calibrated on date and place of calibration.

3. This Certification is traceable to the International System of Unit maintained through:-

- Thunder Scientific Corporation, NVLAB Accreditation No. Calibration 200582-0

- Technology Promotion Association (Thailand-Japan), NSC-ONSC Accredited No. Calibration 0008

Calibrated by : Viporn Tantiyawutti

Issue Date : 17 April 2024

Approved Signatory :

[✓] Chakrit Waeewarajua

[] Viporn Tantiyawutti

[] Unnopphol Harachai

เอกสารไม่ควบคุม

B 0339073



Result of Calibration:-

Without Adjustment

Function: Humidity Measurement.

Reference Temperature (°C)	Standard Humidity (%R.H.)	UUC* Reading (%R.H.)	Error (%R.H.)	Uncertainty of Measurement (±%R.H.)
25.0	40.1	41	0.9	1.3
25.0	50.1	50	-0.1	1.6
25.0	60.0	58	-2.0	1.6
25.0	70.2	66	-4.2	1.6

Result of Calibration:-

Without Adjustment

Function: Temperature Measurement.

Standard Temperature (°C)	UUC* Reading (°C)	Error (°C)	Uncertainty of Measurement (±°C)
19.996	20.3	0.302	0.42
25.031	25.6	0.569	0.42
30.045	30.2	0.155	0.42
40.023	39.9	-0.123	0.42

UUC* : Unit Under Calibration

The reported uncertainty of measurement was base on standard uncertainty multiplied
by coverage factor $k = 2.00$, providing confidence level approximately 95%.

-000-

เอกสารไม่ควบคุม

a 1210371

Certificate of Calibration

Customer : UNITED ANALYST AND ENGINEERING
Name : CONSULTANT CO.,LTD.
Address : 81 Soi Udomsak 41, Sukhumvit Road, Bangchak,
Prakanong, Bangkok 10260

Certificate No : 24-TPM-148
Request No : Req-2024-0540
Page : 1/2

Unit Under Calibration Details

Calibration Parameter : Temperature
Instrument Name : Thermal Environment Monitor
Manufacturer : TSI QUEST
Model : QT-32
Serial Number : TPQ020024
Resolution : 0.1 °C
ID Number : UAE.EFM.007/2559

Range Calibration : 20 °C to 60 °C
Type of Sensor : RTD
Sensor Diameter (mm) : 4.5
Calibration Position (mm) : 67.5
Instrument Status : Used

Calibration Environment and Details

Temperature : 23 °C ± 3 °C
Humidity : 55 %RH ± 15 %RH
Received Date : 5 March 2024
Calibrated Date : 21 March 2024


Calibration Procedure : In-house method CP-TPM-01 by Comparison with Standard Thermometer.

Reference Standard : Digital Thermometer with Sensor, Manufacturer: GINGO GINGO, Model: GT11/ RTD100, SN:
12009077, ID: AR-TPM Which was calibrated on 27 October 2023, Calibration Certificate No. : QR23-
2574

Traceability : This Certificate is traceable to SI Unit through Quality Reborn Co., Ltd., NSC-ONSC Accreditation No.:
Calibration 0292

Note

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor k=2, providing a level of confidence approximately 95 %.

Approved By : 
Mr. Noppadol Luangrat
Technical Manager
Issue Date : 21 March 2024


The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the issuer.
เอกสารไม่ควบคุม

Calibration Note : Certificate No : 24-TPM-148
UUC Adjustment : Not Adjust
Request No : Req-2024-0540
Page : 2/2

Result of Calibration :

UUC Sensor	Standard Temperature (°C)	UUC Reading (°C)	Correction (°C)	Uncertainty (±°C)
WET	20.033	19.0	-0.0	0.13
	25.033	23.0	-0.0	0.13
	30.033	30.0	-0.0	0.13
	35.036	35.0	-0.0	0.13
	40.038	40.0	-0.0	0.13
	45.041	45.0	-0.0	0.13
	50.044	50.0	-0.0	0.13
	60.047	60.0	-0.0	0.13
DRY	20.032	19.9	+0.1	0.13
	25.033	24.9	+0.1	0.13
	30.034	29.9	+0.1	0.13
	35.036	35.0	-0.0	0.13
	40.038	40.0	-0.0	0.13
	45.039	45.0	-0.0	0.13
	50.043	50.0	-0.0	0.13
	60.047	60.0	-0.0	0.13
GLOBE	20.033	19.9	+0.1	0.13
	25.033	24.9	+0.1	0.13
	30.034	29.9	+0.1	0.13
	35.037	35.0	-0.0	0.13
	40.038	40.0	-0.0	0.13
	45.041	45.0	-0.0	0.13
	50.044	50.0	-0.0	0.13
	60.048	60.0	-0.0	0.13

End of Certificate

Calibrated By : 
Mr. Sirinichok Jirapachonkul

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the issuer.
เอกสารไม่ควบคุม

Certificate of Calibration

Customer : UNITED ANALYST AND ENGINEERING
Name : CONSULTANT CO.,LTD.
Address : 81 Soi Udomsak 41, Sukhumvit Road, Bangchak,
Prakanong, Bangkok 10260

Certificate No : 24-TPM-152
Request No : Req-2024-0542
Page : 1/2

Unit Under Calibration Details

Calibration Parameter : Temperature
Instrument Name : Thermal Environment Monitor
Manufacturer : TSI QUEST
Model : QT-32
Serial Number : TPQ020025
Resolution : 0.1 °C
ID Number : UAE.EFM.008/2559

Range Calibration : 20 °C to 60 °C
Type of Sensor : RTD
Sensor Diameter (mm) : 4.5
Calibration Position (mm) : 67.5
Instrument Status : Used

Calibration Environment and Details

Temperature : 23 °C ± 3 °C
Humidity : 55 %RH ± 15 %RH
Received Date : 5 March 2024
Calibrated Date : 21 March 2024


Calibration Procedure : In-house method CP-TPM-01 by Comparison with Standard Thermometer.

Reference Standard : Digital Thermometer with Sensor, Manufacturer: GINGO GINGO, Model: GT11/ RTD100, SN:
12009077, ID: AR-TPM Which was calibrated on 27 October 2023, Calibration Certificate No. : QR23-
2574

Traceability : This Certificate is traceable to SI Unit through Quality Reborn Co., Ltd., NSC-ONSC Accreditation No.:
Calibration 0292

Note

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor k=2, providing a level of confidence approximately 95 %.

Approved By : 
Mr. Noppadol Luangrat
Technical Manager
Issue Date : 21 March 2024

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the issuer.
เอกสารไม่ควบคุม

Calibration Note : Certificate No : 24-TPM-152
UUC Adjustment : Not Adjust
Request No : Req-2024-0542
Page : 2/2

Result of Calibration :

UUC Sensor	Standard Temperature (°C)	UUC Reading (°C)	Correction (°C)	Uncertainty (±°C)
WET	20.050	20.1	-0.1	0.13
	25.053	25.1	-0.1	0.13
	30.055	30.1	-0.1	0.13
	35.056	35.1	-0.1	0.13
	40.058	40.2	-0.2	0.13
	45.061	45.2	-0.2	0.13
	50.064	50.1	-0.2	0.13
	60.067	60.2	-0.2	0.13
DRY	20.051	20.0	0.0	0.13
	25.053	25.0	0.0	0.13
	30.054	30.0	0.0	0.13
	35.056	35.0	0.0	0.13
	40.058	40.1	-0.1	0.13
	45.059	45.1	-0.1	0.13
	50.063	50.1	-0.1	0.13
	60.067	60.1	-0.1	0.13
GLOBE	20.052	20.1	-0.1	0.13
	25.053	25.1	-0.1	0.13
	30.054	30.1	-0.1	0.13
	35.057	35.1	-0.1	0.13
	40.058	40.1	-0.1	0.13
	45.063	45.2	-0.2	0.13
	50.064	50.2	-0.2	0.13
	60.068	60.2	-0.2	0.13

End of Certificate

Calibrated By : 
Mr. Sirinichok Jirapachonkul

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the issuer.
เอกสารไม่ควบคุม

Certificate of Calibration

Customer

Name : UNITED ANALYST AND ENGINEERING
CONSULTANT CO.,LTD.
Address : 81 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Prakanong,
Bangkok 10260

Certificate No : 24-ACT-067
Request No : Req-2024-1024

Unit Under Calibration Details

Measurement item : Acoustic Calibrator
Manufacturer : LARSON DAVIS
Model : CAL150
Serial Number : 6306
ID : UAE.EFM.048/2563
Class : 2
Range : 94 - 114 dB / 1000 Hz
Instrument Status : Used

Calibration Environment and Details

Temperature : (23 ±2 °C)
Humidity : (50 ± 20 %RH)
Barometric Pressure : (1013 ±10.0 hPa)
Received Date : 8 May 2024
Calibration Date : 17 May 2024
Location of Calibration : LAB 1 Acoustic
Calibration Procedure : In-house method CP-ACT-02 based on IEC 60942:2017 Electroacoustics - Sound calibrators


Reference Standard	Model	Serial Number	Traceable	Due Calibration
Sound Calibrator	SV 35A	58079	EEI	31 May 2024
THD Multimeter	2015	1047765	NIMT	16 January 2025

Traceability : This certificate provides traceability of measurement to recognized national standard, and to the realization of the international System of Units (SI).

Note

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor k=2, providing a level of confidence approximately 95 %.

Calibrated By : 
Mr. Noppadon Luangart
Service Calibration Engineer

Approved By : 
Mr. Pacit Mathavorn
Calibration Engineer Supervisor
Issue Date : 17 May 2024

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the head of Calibration Laboratory.
FM-708-ACT-02 Rev.01 Issue date:6/23

เอกสารไม่ควบคุม

Certificate No : 24-ACT-067
Request No : Req-2024-1024

Sound pressure level

Calibration Results : Without Adjustment

Calibration Range (dB)	Without Adjustment (dB)		Adjustment (dB)		Uncertainty (± dB)	Acceptance limit Class 2 (± dB)
	Measured	Deviated value	Measured	Deviated value		
94 dB / 1000 Hz	94.09	0.09	-	-	0.13	0.40
114 dB / 1000 Hz	114.10	0.10	-	-	0.13	0.40

Frequency of Sound pressure level

Calibration Range (Hz)	Without Adjustment		Adjustment		Uncertainty (± %)	Acceptance limit Class 2 (± %)
	Measured (Hz)	Deviated value	Measured (Hz)	Deviated value		
94 dB / 1000 Hz	1000.00	0.00	-	-	0.01	1.7
114 dB / 1000 Hz	1000.00	0.00	-	-	0.01	1.7

Total Harmonic Distortion plus Noise of Sound pressure level (THD+N %)

Calibration Range (Hz)	Without Adjustment		Adjustment		Uncertainty (± %)	Acceptance limit Class 2 (± %)
	Measured (%)	Deviated value	Measured (%)	Deviated value		
94 dB / 1000 Hz	0.05	-	-	-	0.40	3.0
114 dB / 1000 Hz	0.21	-	-	-	0.40	3.0

Note :

Function	Maximum-permitted Uncertainty of measurement
Sound pressure level	0.35 dB
Frequency	0.20%
Total distortion+noise	1.00%

- Acceptance limit was IEC60942:2017 Class 1
- The calibration results exclude the calibrator pressure correction
- The calibration results exclude the microphone volume correction

End of Calibration

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the head of Calibration Laboratory.
FM-708-ACT-02 Rev.01 Issue date:6/23

เอกสารไม่ควบคุม

SITHIPORN ASSOCIATES CO., LTD. CALIBRATION LABORATORY

461-461/1 Sirinthorn Road, Bangbunru, Bangkok, Bangkok, 10700 Thailand
Tel : +66 2433 8331 Email : calibration@sithiporn.com



Cert. No. : ACL24160
Pages : 1 of 8

Calibration Certificate

Equipment : SOUND LEVEL METER
Manufacturer : RION
Model : NL-42 / Microphone UC-52 / Preamplifier NH-24
Serial No.: 00409023 / 185669 / 90468
ID No.: UAE.EFM.011/2564

Condition As Found : GOOD

Customer : UNITED ANALYST AND ENGINEERING CONSULTANT (UAE)
81 SOI UDOMSUK 41, SUKHUMVIT ROAD,
BANGCHAK SUB-DISTRICT,
PHRAKHANONG DISTRICT, BANGKOK 10260
THAILAND.

Location : -
Ambient Temperature : (23.0 ± 3) °C
Pressure : (101.3 ± 3) kPa
Relative Humidity : (50.0 ± 20) %

Received Date : 10 MAY 2024
Calibration Date : 04 - 05 JUNE 2024
Date of Issue : 06 JUNE 2024

Calibrated by : Nathakorn Pisutpaisan

Approved by : 
(Thanakul Petchurai)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

เอกสารไม่ควบคุม

SITHIPORN ASSOCIATES CO., LTD. CALIBRATION LABORATORY

461-461/1 Sirinthorn Road, Bangbunru, Bangkok, Bangkok, 10700 Thailand
Tel : +66 2433 8331 Email : calibration@sithiporn.com



Cert. No. : ACL24160
Job No. : VC67AC0071
Pages : 2 of 8

Calibration Procedure : CP-AC-01

Calibration Method :

This equipment was calibrated by follow on IEC-61672-3 (2013) Standard for sound level meter (SLM). The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.
For tests results of each items were made by observation of each Instruments display and also with SLM's display.

Condition of this result of calibration :

1. Reference Standard Instruments :

Instrument	Model	Serial No.	Cert. No.	Due Date
Waveform Generator	33210A	MY48017076	EF-0009-24	05-FEB-25
Waveform Generator	33511B	MY52302742	EF-0007-24	05-FEB-25
Digital Multimeter	33461A	MY53220104	EEL-BP 21/0267	13-FEB-25
Digital Multimeter	33461A	MY53220076	EEL-BP 20/0267	15-FEB-25
Digital Multimeter	34461A	MY60024273	EEL-BP 22/0267	15-FEB-25
Programmable Attenuator	MAT-1070	62100114	EF-0008-24	05-FEB-25
Condenser Microphone	4180	2977900	AA-1001-24	12-FEB-25
Measuring Amplifier	NA-42KAI	34560495	AA-3001-24	05-FEB-25

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is traceable to the international system of unit maintained at :

- 3.1 National Institute of Metrology (Thailand).
- 3.2 Thailand Institute of Scientific and Technological Research (TISTR).

เอกสารไม่ควบคุม

Summary of Measurement Result :

Parameter	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	0.2	N/A
2. Self-generated noise	0.2	N/A
3. Acoustical signal tests of frequency weightings		
125 Hz	0.3	0.6
1000 Hz	0.3	0.6
8000 Hz	0.3	0.7
4. Electrical signal tests of frequency weightings		
For 10 Hz to 4 kHz	0.3	0.6
For > 4 kHz to 10 kHz	0.3	0.7
For > 10 kHz to 20 kHz	-	1.0
5. Frequency and time weightings at 1 kHz	0.2	0.2
6. Long - term stability	0.1	0.1
7. Level linearity on the reference level range	0.2	0.3
8. Level linearity including the level range control	0.2	0.3
9. Tone burst response	0.2	0.3
10. Peak C sound level	0.2	0.35
11. Overload indication	0.2	0.25
12. High level stability	0.1	0.1

เอกสารไม่ควบคุม

Result of calibration :

1. Absolute sensitivity

Reference Acoustic Signal (dB)	Measured Value (dB)	Deviation (dB)	Acceptance Limit (dB)
93.9 (93.94)	93.9	0.0	±0.3

2. Self-generated noise

2.1 Normal test

Measured Value (dB)
15.6

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Measured value (dB)
A - weight	14.2
C - weight	20.5
Flat	26.0

3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
125	-0.1	-0.1	-0.1	± 1.5
1000	0.0	0.0	0.0	± 1.0
8000	2.0	2.0	2.1	±5.0

เอกสารไม่ควบคุม

4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	-0.1	-0.1	-0.1	±2.0
125	0.0	0.0	-0.1	±1.5
250	0.0	0.0	-0.1	±1.5
500	0.0	0.0	-0.1	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.0	0.0	±2.0
4000	0.0	0.0	0.0	±3.0
8000	0.0	0.0	0.0	±5.0

5. Frequency and time weightings at 1 kHz

5.1 Frequency weightings at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.2
C - weight	94.0	94.0	0.0	± 0.2
Flat	94.0	94.0	0.0	± 0.2

5.2 Time weighting at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	94.0	94.0	0.0	± 0.1
Slow	94.0	94.0	0.0	± 0.1
Leq	94.0	94.0	0.0	± 0.1

6. Long - term stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.2

เอกสารไม่ควบคุม

7. Level linearity on the reference level range

Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
137.0	137.1	0.1	± 1.1
136.0	136.1	0.1	± 1.1
135.0	135.1	0.1	± 1.1
134.0	134.1	0.1	± 1.1
133.0	133.0	0.0	± 1.1
132.0	132.0	0.0	± 1.1
131.0	131.0	0.0	± 1.1
129.0	129.1	0.1	± 1.1
124.0	124.0	0.0	± 1.1
119.0	119.1	0.1	± 1.1
114.0	114.1	0.1	± 1.1
109.0	109.1	0.1	± 1.1
104.0	104.1	0.1	± 1.1
99.0	99.1	0.1	± 1.1
94.0	94.0	0.0	± 1.1
89.0	89.0	0.0	± 1.1
84.0	84.0	0.0	± 1.1
79.0	79.0	0.0	± 1.1
74.0	74.0	0.0	± 1.1
69.0	69.0	0.0	± 1.1
64.0	64.0	0.0	± 1.1
59.0	59.0	0.0	± 1.1
54.0	54.0	0.0	± 1.1
49.0	49.0	0.0	± 1.1
44.0	44.0	0.0	± 1.1
39.0	39.0	0.0	± 1.1
34.0	34.0	0.0	± 1.1
30.0	30.0	0.0	± 1.1
29.0	29.0	0.0	± 1.1
28.0	28.1	0.1	± 1.1
27.0	27.1	0.1	± 1.1
26.0	26.2	0.2	± 1.1
25.0	25.2	0.2	± 1.1

เอกสารไม่ควบคุม

8. Level linearity including the level range control

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Auto	94.0	94.0	0.0	±1.1

9. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Cycle	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.0	0.0	±1.0
Slow	2	8	108.0	108.0	0.0	1.5 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
SEL	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.0	0.0	±1.0

10. Peak C sound level

Number of cycle in test signal	Anticipated Value (dB)	Measured Value, L _{peak} (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	±3.0
One	136.4	136.4	0.0	±3.0

Number of cycle in test signal	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	±2.0
Positive half cycle	135.4	135.1	-0.3	±2.0
Negative half cycle	135.4	135.1	-0.3	±2.0

เอกสารไม่ควบคุม

Calibration Certificate

Equipment : SOUND LEVEL METER
Manufacturer : RION
Model : NL-42 / Microphone UC-52 / Preamplifier NH-24
Serial No.: 00409177 / 185836 / 90623
ID No.: UAE.EFM.016/2564

Condition As Found : GOOD

Customer : UNITED ANALYST AND ENGINEERING CONSULTANT (UAE)
81 SOI UDOMSUK 41, SUKHUMVIT ROAD,
BANGCHAK SUB-DISTRICT,
PHRAKHANONG DISTRICT, BANGKOK 10260
THAILAND.

Location : -
Ambient Temperature : (23.0 ± 3) °C
Pressure : (101.3 ± 3) kPa
Relative Humidity : (50.0 ± 20) %

Received Date : 10 MAY 2024
Calibration Date : 04 - 05 JUNE 2024
Date of Issue : 06 JUNE 2024

Calibrated by : Nuthakorn Pisutpraisan

Approved by : 
(Thanakul Petchurai)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

เอกสารไม่ควบคุม

11. Overload indication

Measured value (dB)		Deviated Value (dB)	Acceptance Limits (dB)
Positive one-half cycle	Negative one-half cycle		
89.6	89.5	-0.1	±1.5

12. High level stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor $k = 2$ or any value following calculation, providing a level of confidence of approximately 95 %

End of Calibration Certificate

เอกสารไม่ควบคุม

Calibration Procedure : CP-AC-01

Calibration Method :

This equipment was calibrated by follow on IEC-61672-3 (2013) Standard for sound level meter (SLM). The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.
For tests results of each items were made by observation of each Instruments display and also with SLM's display.

Condition of this result of calibration :

1. Reference Standard Instruments :

Instrument	Model	Serial No.	Cert. No.	Due Date
Waveform Generator	33210A	MY48017076	EF-0009-24	05-FEB-25
Waveform Generator	33511B	MY52302742	EF-0007-24	05-FEB-25
Digital Multimeter	33461A	MY53220104	EEL-BP 21/0267	13-FEB-25
Digital Multimeter	33461A	MY53220076	EEL-BP 20/0267	15-FEB-25
Digital Multimeter	34461A	MY60024273	EEL-BP 22/0267	15-FEB-25
Programmable Attenuator	MAT-1070	62100114	EF-0008-24	05-FEB-25
Condenser Microphone	4180	2977900	AA-1001-24	12-FEB-25
Measuring Amplifier	NA-42KAI	34560495	AA-3001-24	05-FEB-25

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is traceable to the international system of unit maintained at :

- 3.1 National Institute of Metrology (Thailand),
- 3.2 Thailand Institute of Scientific and Technological Research (TISTR),

Summary of Measurement Result :

Parameter	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	0.2	N/A
2. Self-generated noise	0.2	N/A
3. Acoustical signal tests of frequency weightings		
125 Hz	0.3	0.6
1000 Hz	0.3	0.6
8000 Hz	0.3	0.7
4. Electrical signal tests of frequency weightings		
For 10 Hz to 4 kHz	0.3	0.6
For > 4 kHz to 10 kHz	0.3	0.7
For > 10 kHz to 20 kHz	-	1.0
5. Frequency and time weightings at 1 kHz	0.2	0.2
6. Long - term stability	0.1	0.1
7. Level linearity on the reference level range	0.2	0.3
8. Level linearity including the level range control	0.2	0.3
9. Tone burst response	0.2	0.3
10. Peak C sound level	0.2	0.35
11. Overload indication	0.2	0.25
12. High level stability	0.1	0.1

เอกสารไม่ควบคุม
F. Kellin

4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz:

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	0.0	-0.1	-0.1	±2.0
125	0.0	0.0	0.0	±1.5
250	0.0	0.0	0.0	±1.5
500	0.0	0.0	0.0	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.0	0.0	±2.0
4000	0.0	0.0	0.0	±3.0
8000	0.0	0.1	0.1	±5.0

5. Frequency and time weightings at 1 kHz

5.1 Frequency weightings at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.2
C - weight	94.0	94.0	0.0	± 0.2
Flat	94.0	94.0	0.0	± 0.2

5.2 Time weighting at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	94.0	94.0	0.0	± 0.1
Slow	94.0	94.0	0.0	± 0.1
Loq	94.0	94.0	0.0	± 0.1

6. Long - term stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.1

เอกสารไม่ควบคุม
F. Kellin

Result of calibration :

1. Absolute sensitivity

Reference Acoustic Signal (dB)	Measured Value (dB)	Deviation (dB)	Acceptance Limit (dB)
93.9 (93.94)	93.9	0.0	±0.3

2. Self-generated noise

2.1 Normal test

Measured Value (dB)
16.1

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Measured value (dB)
A - weight	15.1
C - weight	21.6
Flat	27.0

3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
125	0.1	0.1	0.1	± 1.5
1000	-0.1	-0.1	-0.1	± 1.0
8000	1.2	1.3	1.3	±5.0

เอกสารไม่ควบคุม
F. Kellin

7. Level linearity on the reference level range

Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
137.0	137.0	0.0	± 1.1
136.0	136.0	0.0	± 1.1
135.0	135.0	0.0	± 1.1
134.0	134.0	0.0	± 1.1
133.0	133.0	0.0	± 1.1
132.0	132.0	0.0	± 1.1
131.0	131.0	0.0	± 1.1
129.0	129.0	0.0	± 1.1
124.0	124.0	0.0	± 1.1
119.0	119.0	0.0	± 1.1
114.0	114.0	0.0	± 1.1
109.0	109.0	0.0	± 1.1
104.0	104.0	0.0	± 1.1
99.0	99.0	0.0	± 1.1
94.0	94.0	0.0	± 1.1
89.0	89.0	0.0	± 1.1
84.0	84.0	0.0	± 1.1
79.0	79.0	0.0	± 1.1
74.0	74.0	0.0	± 1.1
69.0	69.0	0.0	± 1.1
64.0	64.0	0.0	± 1.1
59.0	59.0	0.0	± 1.1
54.0	53.9	-0.1	± 1.1
49.0	49.0	0.0	± 1.1
44.0	44.0	0.0	± 1.1
39.0	39.0	0.0	± 1.1
34.0	34.0	0.0	± 1.1
30.0	29.9	-0.1	± 1.1
29.0	28.9	-0.1	± 1.1
28.0	27.9	-0.1	± 1.1
27.0	26.9	-0.1	± 1.1
26.0	25.9	-0.1	± 1.1
25.0	25.0	0.0	± 1.1

เอกสารไม่ควบคุม
F. Kellin

8. Level linearity including the level range control

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Auto	94.0	94.0	0.0	±1.1

9. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Cycle	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.0	0.0	±1.0
Slow	2	8	108.0	108.0	0.0	1.5 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
SEL	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.0	0.0	±1.0

10. Peak C sound level

Number of cycle in test signal	Anticipated Value (dB)	Measured Value, L _{peak} (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	±3.0
One	136.4	136.3	-0.1	±3.0

Number of cycle in test signal	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	±2.0
Positive half cycle	135.4	135.2	-0.2	±2.0
Negative half cycle	135.4	135.2	-0.2	±2.0

เอกสารไม่ควบคุม

11. Overload indication

Measured value (dB)		Deviated Value (dB)	Acceptance Limits (dB)
Positive one-half cycle	Negative one-half cycle		
89.6	89.5	-0.1	±1.5

12. High level stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor $k = 2$
or any value following calculation, providing a level of confidence of approximately 95 %

End of Calibration Certificate

เอกสารไม่ควบคุม

List of Instruments Certification for Environmental Quality Analysis

No.	Instrument/Equipment	Parameter	Manufacturer	Model/Serial No.	Calibrator	Certification No.	Date of Calibration	Due date of Calibration*	Remark
Equipment for Air Quality Analysis									
1	Analytical Balance (Readability 0.1 mg)	ฝุ่นละอองรวม (TSP) ฝุ่นขนาดเล็กไม่เกิน 10 ไมครอน (PM10)	Mettler-Toledo	MS204TS/00 C252436235	National Food Institute, Ministry of Industry, Thailand	2402420-003-01	19 Apr 24	18 Apr 25	-
2	Analytical Balance (Readability 0.001 mg)	ฝุ่นทุกขนาด (Total Dust) ฝุ่นขนาดเล็กที่เข้าถึงและสะสมในถุงลมของปอดได้ (Respirable dust)	Mettler-Toledo	XP6 / B322373893	National Food Institute, Ministry of Industry, Thailand	2402420-002-01	19 Apr 24	18 Apr 25	-
3	UV-VIS Spectrophotometer	ก๊าซไนโตรเจนไดออกไซด์ (NO2)	Hitachi	U-5100 / 23A4-008	DOE Services Co.,Ltd.	SP24-028	10 Sep 24	9 Sep 25	-
Equipment for Water Quality Analysis									
4	pH Meter	ความเป็นกรดและด่าง (pH) อุณหภูมิ (Temp)	Mettler-Toledo	Seven Easy S20 / 1231155210	National Food Institute, Ministry of Industry, Thailand	2401718-001-01	11 Mar 24	10 Mar 25	-
5	pH Meter		Mettler-Toledo	Seven Easy S20 / 1230525212	DKSH (Thailand) Ltd.	C07240167	9 Apr 24	8 Apr 25	-
6	Analytical Balance (Readability 0.1 mg)	น้ำมันและไขมัน (Oil & Grease)	Mettler-Toledo	XSR204 / C117635043	Technology Promotion Association (Thailand-Japan)	24MM293	11 May 24	10 May 25	-
7	Analytical Balance (Readability 0.01 mg)	ของแข็งละลายน้ำทั้งหมด (TDS) ของแข็งแขวนลอยทั้งหมด (TSS)	Mettler-Toledo	XSR205DU / C210685394	National Food Institute, Ministry of Industry, Thailand	2402283-002-01	2 Apr 24	1 Apr 25	-
8	Hot Air Oven		Memmert	UF55 / B216.1666	National Food Institute, Ministry of Industry, Thailand	2500116-001-01	8 Oct 24	7 Oct 25	-
9	UV-VIS Spectrophotometer	ซัลเฟต (Sulphate), ไซยาไนด์ (Cyanide), สี (Color) ไนเตรท ในรูปของเตรท (Nitrate), ฟีนอล (Phenol) แอมโมเนีย ในหน่วยไนโตรเจน (Ammonia-Nitrogen) ฟอร์มิลดีไฮด์ (Formaldehyde), ซีโอดี (COD)	Agilent Technologies	Cary60 G6860A / MY15410009	DOE Services Co.,Ltd.	SP24-018	7 May 24	6 May 25	-
10	UV-VIS Spectrophotometer	การนำไฟฟ้า (EC)	Hitachi	U-5100 / 23A4-008	DOE Services Co.,Ltd.	SP24-028	10 Sep 24	9 Sep 25	-
11	Conductivity Meter		Mettler-Toledo	SevenDirect SD30/ C441872132	DKSH (Thailand) Ltd.	C24250010	15 Jan 25	14 Jan 26	-
12	BOD Incubator	บีโอดี (BOD) ออกซิเจนละลาย (DO)	Arco	UC4-1320 / (UAE.WAO.018/2559)	Technology Promotion Association (Thailand-Japan)	24TM1114	11 Jul 24	10 Jul 25	-
13	DO Meter		YSI	4010-2W / 20260326	Technology Promotion Association (Thailand-Japan)	24TW222	17 Oct 24	16 Oct 25	-

List of Instruments Certification for Environmental Quality Analysis

No.	Instrument/Equipment	Parameter	Manufacturer	Model/Serial No.	Calibrator	Certification No.	Date of Calibration	Due date of Calibration*	Remark
14	COD Reactor (Heating Block)	ซีโอดี (COD)	Hanna	HI839800 / 1147807	Hanna Instruments (Thailand) Ltd.	HIT-2417-0568	25 Apr 24	24 Apr 25	-
15	Atomic Absorption Spectrophotometer (AAS)	สารหนู (As), ปปรอท (Hg), ทองแดง (Cu), ตะกั่ว (Pb) นิกเกิล (Ni), แบเรียม (Ba), แคดเมียม (Cd), แมงกานีส (Mn) โครเมียม (Cr), ซีลีเนียม (Se), สังกะสี (Zn)	Perkin Elmer	PinAAcle 900F / PFBS20031902	Perkin Elmer Co.,Ltd.	PinAAcle 900F	14 May 24	13 May 25	-
16	Inductively Coupled Plasma (ICP)	โครเมียมเฮกซะวาเลนท์ (Cr6+) โครเมียมไตรวาเลนท์ (Cr3+)	Agilent Technologies	System ID:G8015A G8015AA / MY18030001	Agilent Technologies (Thailand) Co.,Ltd.	Preventive Maintenance Checklist	4 Nov 24	3 Nov 25	-
17	Cold Vapor Atomic Absorption (CVAAS)	ปรอท (Hg)	Nippon Instrument Corporation	RA-4500 / 17780278	Coax Group Corporation Ltd.	Preventive Maintenance Report	9 Jul 24	8 Jul 25	-
18	Digestor Unit	ทีเคเอ็น (TKN)	FOSS TECATOR	DT2520 / 91794469	National Food Institute, Ministry of Industry, Thailand	2402957-001-01	23 May 24	22 May 25	-
19	Distillation Unit (Kjeldahl Method)		FOSS TECATOR	KT200 / 91790524	FOSS South East Asia	13319	27 Jan 25	26 Jan 26	-
20	Gas Chromatography (GC)	อัลฟา-บีเอพซี (Alpha-BSC), เบต้า-บีเอพซี (Bata-BSC) แกมมา-บีเอพซี (Gamma-BSC), เดลต้า-บีเอพซี (Delta-BSC) อัลดริน (Aldrin), ดิลดริน (Dieldrin) , เอนได์ซิลแฟน (I) (Endosulfan I)), เอนได์ซิลแฟน (II), (Endosulfan (II)) เอนได์ซิลแฟน ซัลเฟต (Endosulfan Sulfate) เอนดริน (Endrin), เอนดริน อีตี่เฮต์ (Endrin Aldehyde)	Agilent Technologies	System ID:CN13113001 7890 / CN13113001	Agilent Technologies (Thailand) Co.,Ltd.	Preventive Maintenance Checklist	17 Apr 24	16 Apr 25	-
21	Gas Chromatography - Mass Spectrometer (GC-MS)	เฮปตาคลอร์ (Heptachlor), ออโร,พารา-ดีดีอี (o,p'-DDE) เฮปตาคลอร์ อีปอกไซด์ (Heptachlor Epoxide) เมท็อกซีคลอร์ (Methoxychlor) พารา,พารา-ดีดีดี (p,p'-DDD), พารา,พารา-ดีดีที (p,p'-DDT)	Bruker Scion	451-GC / BR1201M099 Scion-SQ / GQS1203F021 CP8400 / BR1203M331	Thai Unique Co.,Ltd.	SV2407/21898	16 Jul 24	15 Jul 25	-
22	Gas Chromatography - Mass Spectrometer (GC-MS)		Agilent Technologies	System ID: US2009M037 8890 (G3542A) / CN1945A066 5977B / US2009M037	Agilent Technologies (Thailand) Co.,Ltd.	Preventive Maintenance Checklist	27 May 24	26 May 25	-

List of Instruments Certification for Environmental Quality Analysis

No.	Instrument/Equipment	Parameter	Manufacturer	Model/Serial No.	Calibrator	Certification No.	Date of Calibration	Due date of Calibration*	Remark
23	Incubator	แบคทีเรียกลุ่มโคลิฟอร์มทั้งหมด (Total Coliform Bacteria)	Binder	KB400 / 20200000015535	Technology Promotion Association (Thailand-Japan)	24TM647	1 Apr 24	31 Mar 25	-
24	Incubator		Memmert	IPP 260 / V616.0066	Technology Promotion Association (Thailand-Japan)	24TM650	2 Apr 24	1 Apr 25	-
25	Water Bath		Memmert	WNE 14 / L414.1407	Technology Promotion Association (Thailand-Japan)	24TM614	1 Apr 24	31 Mar 25	-
26	Water Bath		Memmert	WNE 14 / L414.1410	Technology Promotion Association (Thailand-Japan)	24TM616	1 Apr 24	31 Mar 25	-
27	Auto Clave		ALP	CL-40L / 807298	National Food Institute, Ministry of Industry, Thailand	2403982-001-01	7 Aug 24	6 Aug 25	-
28	Auto Clave		ALP	CL-40L / 808763	National Food Institute, Ministry of Industry, Thailand	2402281-001-01	2 Apr 24	1 Apr 25	-
29	Analytical Balance		OHAUS	PX623 / C236754745	DKSH (Thailand) Ltd.	<u>2402419-001-01</u>	19 Apr 24	18 Apr 25	-

Due Date of Calibration* : Based on the annual calibration plan. At least 1 time per year.

Calibration Certificate

Certificate No.: 2402420-003-01
Client name: UNITED ANALYST AND ENGINEERING CONSULTANT CO., LTD.
Address: 3 Soi Udomsuk 41, Sukhumvit Road,
Bangchack, Prakhonong, Bangkok 10260

Page 1 of 3

Equipment: Electronic Balance
Manufacturer: METTLER TOLEDO
Model: MS204TS/00
Serial No.: C252436235
ID No.: UAE.AIR.023/2566
Order No.: 2402420
Operation No.: 2402420-003
Date of Receipt: 19 April 2024
Date of Calibration: 19 April 2024

Calibrated by Mr. Pheraphat Tuanjit
Scientist
Approved by P. Jaengbanchit
(Miss Preeyaporn Jaengkarnkit)
Vice President, Department of Laboratory Services
Responsible for the Technical Management Team
Date of Issue: 23 April 2024

The uncertainties are for a confidence probability of approximately 95%

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the National Food Institute.

F-CS-009 Revision: 01 Date: 20-04-65

Calibration Report

Certificate No.: 2402420-003-01
Equipment: Electronic Balance
Manufacturer: METTLER TOLEDO
Model: MS204TS/00
Serial No.: C252436235
Capacity: 220 g
Resolution: 0.0001 g
ID No.: UAE.AIR.023/2566

Page 2 of 3

Date of Calibration: 19 April 2024

Environment Condition: Ambient Temperature: 21.7 ± 1.5 °C Relative Humidity: 65 ± 6.7 %

Place of Calibration: Room 206 Balance Room 2, UNITED ANALYST AND ENGINEERING CONSULTANT CO., LTD.

Condition of Equipment: Good Condition

Condition of This Results of Calibration:

1. Calibration Method: NFI Method W-MA-001 In-House Method based on UKAS Lab 14 : 2019

2. Reference Standards:

Reference Standard	Model	Serial No.	Calibrated By	Certificate No.	Due Date
Standard Weight Class E2	1-500mg	15880	TCS	M23111815	28 November 2024
Standard Weight Class E2	1-500g	15882	TCS	M23111825	28 November 2024

Instrument	Model	Serial No.	Calibrated By	Certificate No.	Due Date
Thermo-Hygro Meter	608-H1	NFLBTH 019/23	Quality Return	QR24-0492	4 March 2025

3. This certification is traceable to SI UNIT

4. This certificate was certified only for the instrument we calibrated.

5. This result of calibration was found accurate as shown on date and place of calibration only.

Calibration Results:

1. Repeatability of Reading:

Nominal Value (g)	Standard Deviation of Reading (g)
100	0.000074
200	0.000074

2. Off-Center Error:

A mass of 100 g was placed and moved to various position on pan.

The balance reading obtained is given in the table:

1	2	3	4	5	6	(Maximum Difference)
(g)	(g)	(g)	(g)	(g)	(g)	(g)
100.0005	100.0006	100.0003	100.0006	100.0003	100.0005	0.0002

F-CS-012 Revision: 01 Date: 20-04-65

Calibration Report

Certificate No.: 2402420-003-01
Equipment: Electronic Balance
Manufacturer: METTLER TOLEDO
Model: MS204TS/00
Serial No.: C252436235
Capacity: 220 g
Resolution: 0.0001 g
ID No.: UAE.AIR.023/2566

Date of Calibration: 19 April 2024

Calibration Results: (Continued)

Calibration Range: 0-200 g

Calibration Adjustment: Internal Calibration

3. Departure from Nominal Value:

Nominal Value (g)	Standard Value (g)	Average Reading (g)	Correction (g)	Uncertainty (g)	Coverage Factor #
Unload	0.00000	0.0000	0.0000	0.000094	2.00
0.1	0.10000	0.1000	0.0000	0.000094	2.00
1	0.99998	1.0000	0.0000	0.000097	2.00
5	4.99997	5.0000	0.0000	0.000096	2.00
10	10.00002	10.0000	0.0000	0.00012	2.00
20	20.00003	20.0001	-0.0001	0.00014	2.00
50	49.99998	50.0003	-0.0003	0.00012	2.00
70	70.00000	70.0005	-0.0005	0.00017	2.00
100	99.99997	100.0006	-0.0006	0.00017	2.00
150	149.99994	150.0012	-0.0013	0.00022	2.00
200	200.00001	200.0015	-0.0015	0.00028	2.00

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k, providing a level of confidence of approximately 95 %.

F-CS-012 Revision: 01 Date: 20-04-65

Calibration Certificate

Certificate No.: 2402420-002-01
Client name: UNITED ANALYST AND ENGINEERING CONSULTANT CO., LTD.
Address: 3 Soi Udomsuk 41, Sukhumvit Road,
Bangchack, Prakhonong, Bangkok 10260

Page 1 of 3

Equipment: Electronic Balance
Manufacturer: METTLER TOLEDO
Model: XP6
Serial No.: B322373893
ID No.: UAE.AIR.019/2556
Order No.: 2402420
Operation No.: 2402420-002
Date of Receipt: 19 April 2024
Date of Calibration: 19 April 2024

Calibrated by Mr. Pheraphat Tuanjit
Scientist
Approved by P. Jaengbanchit
(Miss Preeyaporn Jaengkarnkit)
Vice President, Department of Laboratory Services
Responsible for the Technical Management Team
Date of Issue: 23 April 2024

The uncertainties are for a confidence probability of approximately 95%

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the National Food Institute.

F-CS-009 Revision: 01 Date: 20-04-65

DQE Services Co.,Ltd. 32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Bangkok 10230 Phone : +66 (0)2 538 2054, Email : dqeservicesinfo@gmail.com

REPORT OF CALIBRATION

Certificate No. : SP24-028 Page 3 of 5

Calibration Results : Without adjustment

Photometric Accuracy :

Wavelength (nm.)	CRMs Values (Abs)	UUC Reading (Abs)	Correction (Abs)	Uncertainty (Abs)	Coverage factor k
420	0.0000	0.000	0.0000	0.0028	2.00
	0.5780	0.575	0.0030	0.0031	2.00
	1.0484	1.044	0.0044	0.0029	2.00
	2.1876	2.190	-0.0024	0.0075	2.00
440	0.0000	0.000	0.0000	0.0028	2.00
	0.5595	0.557	0.0025	0.0034	2.00
	1.0239	1.021	0.0029	0.0035	2.00
	2.1230	2.121	0.0020	0.0079	2.00
465	0.0000	0.000	0.0000	0.0028	2.00
	0.5230	0.519	0.0040	0.0029	2.00
	0.9633	0.961	0.0023	0.0028	2.00
	1.9753	1.975	0.0003	0.0070	2.00
546.1	0.0000	0.000	0.0000	0.0028	2.00
	0.5181	0.515	0.0031	0.0031	2.00
	1.0002	0.997	0.0032	0.0033	2.00
	1.9973	1.996	0.0013	0.0085	2.00
590	0.0000	0.000	0.0000	0.0028	2.00
	0.5517	0.549	0.0027	0.0030	2.00
	1.0803	1.078	0.0023	0.0029	2.00
	2.0373	2.031	0.0063	0.0081	2.00
635	0.0000	0.000	0.0000	0.0028	2.00
	0.5591	0.557	0.0021	0.0031	2.00
	1.0518	1.049	0.0028	0.0029	2.00
	1.9274	1.923	0.0044	0.0080	2.00

เอกสารไม่ควบคุม
FM-708-02 R01 1/11/2021

DQE Services Co.,Ltd. 32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Bangkok 10230 Phone : +66 (0)2 538 2054, Email : dqeservicesinfo@gmail.com

REPORT OF CALIBRATION

Certificate No. : SP24-028 Page 4 of 5

Photometric Accuracy :

Wavelength (nm.)	CRMs Values (Abs)	UUC Reading (Abs)	Correction (Abs)	Uncertainty (Abs)	Coverage factor k
235	0.0000	0.000	0.0000	0.0050	2.00
	0.7469	0.743	0.0039	0.0056	2.00
257	0.0000	0.000	0.0000	0.0050	2.00
	0.8674	0.862	0.0054	0.0059	2.00
313	0.0000	0.000	0.0000	0.0050	2.00
	0.2919	0.291	0.0009	0.0051	2.00
350	0.0000	0.000	0.0000	0.0050	2.00
	0.6430	0.639	0.0040	0.0055	2.00

เอกสารไม่ควบคุม
FM-708-02 R01 1/11/2021

DQE Services Co.,Ltd. 32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Bangkok 10230 Phone : +66 (0)2 538 2054, Email : dqeservicesinfo@gmail.com

REPORT OF CALIBRATION

Certificate No. : SP24-028 Page 5 of 5

Wavelength Accuracy :

CRMs Values (nm.)	UUC Reading (nm.)	Correction (nm.)	Uncertainty (nm.)	Coverage factor k
241.00	240.4	0.60	0.18	2.00
279.30	278.7	0.60	0.18	2.00
288.90	288.5	0.40	0.18	2.00
334.50	334.2	0.30	0.18	2.00
361.40	361.1	0.30	0.18	2.00
418.40	418.0	0.40	0.18	2.00
447.20	446.7	0.50	0.18	2.00
459.30	459.6	-0.30	0.18	2.00
537.00	536.6	0.40	0.18	2.00
638.00	637.4	0.60	0.18	2.00
441.29	440.8	0.49	0.18	2.00
479.88	479.6	0.28	0.18	2.00
513.75	513.5	0.25	0.18	2.00
528.59	528.6	-0.01	0.18	2.00
575.10	574.9	0.20	0.18	2.00
585.56	585.3	0.26	0.20	2.00
684.70	684.1	0.60	0.18	2.00
740.51	740.0	0.51	0.20	2.00
747.61	747.2	0.41	0.18	2.00
807.04	806.3	0.74	0.18	2.00
879.68	878.9	0.78	0.18	2.00

Remark : - UUC = Unit Under Calibration

- N/A = Not Available

- The result expanded uncertainty of measurement U is stated as the standard uncertainty of measurement multiplied by the coverage factor k.

which for a normal distribution corresponds to a coverage probability of approximately 95%

- End of Certificate -

เอกสารไม่ควบคุม
FM-708-02 R01 1/11/2021

Calibration Certificate

Certificate No.: 2401718-001-01
Client name: UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.
Address: 3 Soi Udomsuk 41, Sukhumvit Road, Bangchack, Prakhonong, Bangkok 10260

Equipment: pH Meter
Manufacturer: METTLER TOLEDO
Model: SevenEasy pH
Serial No.: 1231156210
ID No.: UAE.WAT.010/2553
Order No.: 2401718
Operation No.: 2401718-001
Date of Receipt: 27 February 2024
Date of Calibration: 11 March 2024

Calibrated by Mr.Manas Somsak Specialist
Approved by (Mr.Pheraphat Tuanjit) Manager, Division of Calibration Laboratory
Date of Issue: 12 March 2024
Responsible for the Technical Management Team

The uncertainties are for a confidence probability of approximately 95%.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the National Food Institute.

F-CS-009 Revision: 01 Date: 20-04-65

เอกสารไม่ควบคุม
3208 Soi 35, Anan Asoke Road, Bang Phai Subdistrict, Bang Phai District, Bangkok 10710, Thailand
Tel : +66(0)2 538 2054 Fax : +66(0)2 538 2055



Certificate of Calibration

Equipment: pH METER
Model: SevenEasy
Serial No. (or ID.): 1230525212 (UAE.WAS.003/2553)
Manufacturer: METTLER TOLEDO
Electrode Serial No.: 1156883
Condition: In Condition

Certificate No.: C07240167
Issued Date: 9 April 2024
Job No.: WO-00024208
Page: 1 of 3

Customer: United Analyst and Engineering Consultant Company Limited
3 Soi Udomsuk 41 Sukhumvit Road,
Bangkok, Prakanong, Bangkok 10260 Thailand

Environment Condition: Temperature 23 °C ± 2 °C
Humidity 50 %RH ± 15 %RH

Calibration Place: Environment Laboratory, DKSH Technology Limited,
2533 Sukhumvit Road, Bangkok,
Phrakhanong, Bangkok 10260 Thailand

Calibration By: Miss.Orawan Khlaiphloi

Calibration Date: 9 April 2024

The Method used: In house method, CAL-WI-58, base on ASTM E 70-07

Traceability: This certificate is traceable to SI Units, Sample Test is assured through primary measurement method Hamed cell, through CPAchem Ltd. (ISO/IEC 17034) Certificate No. 938377, 931985, 931984 And pH Scale traceable to the SI Units maintained by National Institute of Metrology (NIMT), Thailand through Industrial Foundation Electrical and Electronics Institute Certificate No. CA20230350EA

Calibration Results:

pH Scale

Input	pH Meter Reading			Uncertainty of Measurement (mV)	Coverage Factor (k)
	(mV)	Error (mV)	(pH)		
414.12	414	-0.12	0.00	0.58	2.00
354.96	355	0.04	1.00	0.58	2.00
295.8	296	0.20	2.00	0.58	2.00
236.64	237	0.36	3.00	0.58	2.00
177.48	178	0.52	4.00	0.58	2.00
118.32	118	-0.32	5.00	0.58	2.00
59.16	59	-0.16	6.00	0.58	2.00
0	0	0.00	7.00	0.58	2.00
-59.16	-59	0.16	8.00	0.58	2.00
-118.32	-118	0.32	9.00	0.58	2.00
-177.48	-177	0.48	10.00	0.58	2.00
-236.64	-236	0.64	11.00	0.58	2.00
-295.8	-296	-0.20	12.00	0.58	2.00
-354.96	-355	-0.04	13.00	0.58	2.00
-414.12	-414	0.12	14.00	0.58	2.00

Orawan Khlaiphloi

(Miss Orawan Khlaiphloi)
Person in charge

Nitinun Sthawan

(Mr. Nitinun Sthawan)
Authorized signatory

This certificate is issued the units of measurement according to the International System of Units (SI). It provides traceability of measurement to international or national standard or other recognized national standard laboratories.

The measurement uncertainty stated is the expanded uncertainty which is obtained from the standard uncertainty multiplied by the coverage factor (k=2) to provide a level of confidence of approximately 95%. It is determined in accordance with the Guide to Expression of Uncertainty in Measurement (GUM).

These results may be affected by deviations from specified conditions. The results relate only to the items tested, calibrated or sampled. The report shall not be reproduced except in full without approval of DKSH Technology Limited.

บริษัท ดีเคเอส อีเซีย จำกัด
DKSH Technology Limited
2533 ซอยสุขุมวิท 41 แขวงคลองเตยใหม่ เขตปทุมธานี 10260
2533 Sukhumvit Road, Bangkok, Phrakhanong, Bangkok 10260
Phone: +66 2639 7000 Email: info.calibration@dksh.com Website: www.dksh.com/scientific-thailand

Delivering Growth - in Asia and Beyond.

เอกสารไม่ควบคุม
CAL-FM-C07-14: 9 Apr 2024

บริษัท ดีเคเอส อีเซีย จำกัด
DKSH Technology Limited
2533 ซอยสุขุมวิท 41 แขวงคลองเตยใหม่ เขตปทุมธานี 10260
2533 Sukhumvit Road, Bangkok, Phrakhanong, Bangkok 10260
Phone: +66 2639 7000 Email: info.calibration@dksh.com Website: www.dksh.com/scientific-thailand

Delivering Growth - in Asia and Beyond.

เอกสารไม่ควบคุม
CAL-FM-C07-14: 9 Apr 2024



Practical slope and zero point*

The three-point calibration using three standard buffer solutions; pH 4.008 , pH 6.985 and pH 9.997

-During calibration, display of pH meter reading: pH 4.00 , pH 7.00 and pH 10.01

The practical slope of the pH electrode; 57.01 (mV/pH), 96.37%

The zero point of the pH electrode; 6.88 (pH)

Sample Test Results

Standard Buffer Solution (pH)	Unit Under Calibration (pH)	Difference (pH)	Uncertainty of Measurement (pH)	Coverage Factor (k)
4.008	3.99	-0.018	0.0070	2.00
6.985	7.00	0.015	0.0091	2.00
9.997	10.02	0.023	0.0074	2.00

* Calibration Marked * Not TISI Accredited * in this Certificate have been included for completeness.

The End of Certificate



Certificate of Calibration

Equipment: Digital Thermometer with Probe
Model: SevenEasy pH
Serial No.: 1230525212
Manufacturer: METTLER TOLEDO
ID No.: UAE.WAS.003/2553

Certificate No.: C15240373
Issued Date: 09 April 2024
Job No.: WO-00024208
Page: 1 of 2
Condition: In Condition

Customer: United Analyst and Engineering Consultant Company Limited
3 Soi Udomsuk 41 Sukhumvit Road,
Bangkok, Prakanong, Bangkok 10260 Thailand

Environment Condition: Temperature: 22 °C ± 3 °C
Humidity: 50 %RH ± 20 %RH
Voltage: 220 VAC ± 10 %

Calibration Place: Thermo-Hygro Laboratory, DKSH Technology Limited,
2533 Sukhumvit Road, Bangkok,
Phrakhanong, Bangkok 10260 Thailand

Calibration By: Mr. Nateekarn Mitjit

Calibration Date: 09 April 2024

The Method used: In house method, CAL-WI-19, by comparison with standard thermometer

Traceability: This certificate is traceable to the International System of Unit maintained by Quality Reborn Co.,Ltd. (QR) Certificate No. QR23-1073

Nateekarn Mitjit

(Mr. Nateekarn Mitjit)
Person in charge

Pramote Ramrong

(Mr. Pramote Ramrong)
Authorized signatory

This certificate is issued the units of measurement according to the International System of Units (SI). It provides traceability of measurement to international or national standard or other recognized national standard laboratories.

The measurement uncertainty stated is the expanded uncertainty which is obtained from the standard uncertainty multiplied by the coverage factor (k=2) to provide a level of confidence of approximately 95%. It is determined in accordance with the Guide to Expression of Uncertainty in Measurement (GUM).

These results may be affected by deviations from specified conditions. The results relate only to the items tested, calibrated or sampled. The report shall not be reproduced except in full without approval of DKSH Technology Limited.

บริษัท ดีเคเอส อีเซีย จำกัด
DKSH Technology Limited
2533 ซอยสุขุมวิท 41 แขวงคลองเตยใหม่ เขตปทุมธานี 10260
2533 Sukhumvit Road, Bangkok, Phrakhanong, Bangkok 10260
Phone: +66 2639 7000 Email: info.calibration@dksh.com Website: www.dksh.com/scientific-thailand

Delivering Growth - in Asia and Beyond.

เอกสารไม่ควบคุม
CAL-FM-C15-14: 08 Dec 2022

บริษัท ดีเคเอส อีเซีย จำกัด
DKSH Technology Limited
2533 ซอยสุขุมวิท 41 แขวงคลองเตยใหม่ เขตปทุมธานี 10260
2533 Sukhumvit Road, Bangkok, Phrakhanong, Bangkok 10260
Phone: +66 2639 7000 Email: info.calibration@dksh.com Website: www.dksh.com/scientific-thailand

Delivering Growth - in Asia and Beyond.

เอกสารไม่ควบคุม
CAL-FM-C15-14: 08 Dec 2022

Reference standard equipment:

Equipment	Certificate no	Cal. date	Next Cal. date
Digital Thermometer with Probe	QR23-1073	2 May 23	2 May 24

Calibration Results:

Without Adjustment

Sensor Type: RTD

Channel: -

Diameter (mm) 4

Length (mm): 135

Immersion (mm): 110

Calibrate Point (°C)	STD. Reading (°C)	UUC. Reading (°C)	Correction of UUC (°C)	Uncertainty (± °C)
15.0	15.010	15.1	-0.090	0.076
25.0	25.006	25.1	-0.094	0.076
35.0	35.004	35.0	0.004	0.076

The End of Certificate

บริษัท ดีเคเอส อีเซีย จำกัด
DKSH Technology Limited
2533 ถนนสุขุมวิท แขวงคลองเตย เขตคลองเตย กรุงเทพมหานคร 10110
2533 Sukhumvit Road, Bangkok, Phrakhanong, Bangkok 10110
Phone: +66 2639 7000 Email: info.calibration@dksh.com Website: www.dksh.com/scientific-thailand

Delivering Growth - in Asia and Beyond.

เอกสารไม่ควบคุม
CAL-FM-C15-14; 06 Dec 2022

TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL 0-2717-3000-29 FAX 0-2719-9484



Certificate of Calibration

Cert.No.: 24MM293
Page: 1 of 3

Equipment : Electronic Balance
Manufacturer : Mettler Toledo
Model : XSR204
Serial No. : C117635043
ID No. : UAE.WAS.012/2564
Submitted by : United Analyst and Engineering Consultant Co.,Ltd.
3 Soi Udomsuk 41, Sukhumvit Road,
Bangchak, Phrakhanong,
Bangkok 10260
Location : Balance Room (108)
Received order : 11 May 2024
Calibration Date : 11 May 2024
Ambient Temperature : 15 °C to 40 °C
Relative Humidity : 30 % to 90 %
Calibrated by : Khit Ruttanaprapachai
Approved by :
() Ponpan Paipim
() Suwit Imjai
(✓) Kunchit Promprat

Issue Date : 15 May 2024

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3: Equipment Calibration and Testing Services.

เอกสารไม่ควบคุม



Equipment : Electronic Balance
Condition As-Received : Used Item
Reference : 2405-0166OC-2

Cert.No.: 24MM293
Page: 2 of 3

Procedure used :-

Calibration were conducted using in-house calibration procedure CP-OB01 based on UKAS LAB 14
according to direct measurement method against standard weight.

Condition of this result of calibration

1. Reference standard instruments:-

- | Instruments | Model | Serial No. | ID No. | Test report No. | Due date |
|-----------------------------|-------|------------|---------|-----------------|-------------|
| 1) Standard Weight Set (E2) | 15884 | 24053 | 70RC007 | MM-0013-24 | 25 Jan 2026 |
- This certificate is valid only to the item calibrated on date and place of calibration.
 - This result of calibration was made on requested at the point specified by customer.
 - This certificate is not certified for any commercial transaction.
 - This certification is traceable to the International System of Unit.

Result of calibration () Without Adjustment (*) After Adjustment by Internal Calibration

Range capacity : 0 g to 220 g Resolution 0.0001 g

Before Adjustment :

Applied Weight	Balance Reading	Correction	Measurement Uncertainty	Coverage Factor
(g)	(g)	(g)	(± mg)	(k)
100	100.0000	0.0000	0.27	2.03
200	200.0001	-0.0001	0.31	2

After Adjustment :

1. Determination of the standard deviation of weighing machine (n = 10)

Applied Weight	Standard Deviation of Reading (g)
(g)	
100	0.00007
200	0.00007




Equipment : Electronic Balance
Condition As-Received : Used Item
Reference : 2405-0166OC-2

Cert.No.: 24MM293
Page: 3 of 3

Result of calibration

2. Effect of off center loading

A mass of 100 g was placed to various position on the pan.
The weighing machine reading error obtained is given in the table

Maximum difference between
off-center and central loading
(g)
0.0003

Position 1	Position 2	Position 3	Position 4	Position 5
(g)	(g)	(g)	(g)	(g)
+0.0002	-0.0001	0.0000	+0.0002	0.0000

3. Departure from nominal value

Applied Weight	Balance Reading	Correction	Measurement Uncertainty	Coverage Factor
(g)	(g)	(g)	(± mg)	(k)
Unload	0.0000	0.0000	0.15	2.13
1	1.0000	0.0000	0.15	2.13
5	5.0000	0.0000	0.15	2.13
10	10.0000	0.0000	0.15	2.11
20	20.0000	0.0000	0.19	2.03
50	50.0001	-0.0001	0.19	2.06
60	60.0001	-0.0001	0.19	2.04
80	80.0001	-0.0001	0.27	2
100	100.0002	-0.0002	0.27	2.03
120	120.0001	-0.0001	0.29	2
200	200.0001	-0.0001	0.31	2

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k, providing a level of confidence of approximately 95 %.

-000-

เอกสารไม่ควบคุม

เอกสารไม่ควบคุม

Calibration Certificate

Certificate No.: 2500116-001-01
Client name: UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.
Address: 3 Soi Udomsuk 41, Sukhumvit Road,
Bangchack, Prakhonong, Bangkok 10260

Page 1 of 3

Equipment: CHAMBER (Hot Air Oven)
Manufacturer: MEMMERT
Model: UF55
Serial No.: B216.1666
ID No.: UAE.WAO.027/2559
Order No.: 2500116
Operation No.: 2500116-001
Date of Receipt: 8 October 2024
Date of Calibration: 8 October 2024

Calibrated by Mr.Yuthin Charoensuk
Scientist
Approved by (Mr.Pheraphat Tuanjit)
Manager, Division of Calibration Laboratory
Responsible for the Technical Management Team
Date of Issue: 15 October 2024

The uncertainties are for a confidence probability of approximately 95 %.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the National Food Institute.

F-C5-002 Revision: 01 Date: 20-04-65

เอกสารไม่ควบคุม เอกสารไม่ควบคุม

Calibration Report

Certificate No.: 2500116-001-01
Equipment: CHAMBER (Hot Air Oven)
Model: UF55 Serial No.: B216.1666
Resolution: 0.1 °C ID No.: UAE.WAO.027/2559
Manufacturer: MEMMERT

Date of Calibration: 8 October 2024

Page 2 of 3

Location: Laboratory, UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.
Environment Condition: Ambient Temperature (30.3 ± 1) °C
Relative Humidity (55 ± 1) %
Line Voltage (230 ± 3) Volt

Condition of this results of Calibration:

- This instrument was calibrated by insert 9 standard thermometer into its chamber and calibration according to W-TE-014 Based on TIAS G-20-1/02-08 (E): Guidelines for Calibration and Checks of Temperature Controlled Enclosures.
- The temperature scale used was based on ITS - 90.
- All data show below were final values and the initial data may be obtained upon request.

2. Reference Standard Instrument :

Instrument	Model	Serial No./ID No.	Certificate No.	Due Date	Through
Digital Thermometer with sensor	34972A	MY57003188	TE 670486-01	8 June 2025	NATIONAL FOOD INSTITUTE
	RTD	CH201-209; RTD#201-209			

- This certificate is traceable to International System of Units (SI Units).

- This certificate was certified only for the instrument we calibrated.

- This result of calibration was found accurate as shown on date and place of calibration only.

- Condition of Calibrated item : Good

UUC Description :

Time of Record 1 Hour 9 Minute At 104.0,140.0 and 180.0 °C
Fresh air Damper - Open Position - 40%
- X Close Fan 40%
- Not Available

- Result of Calibration : X Without adjustment After adjustment

F-C5-012 Revision: 01 Date: 20-04-65

เอกสารไม่ควบคุม เอกสารไม่ควบคุม

Calibration Report

Certificate No.: 2500116-001-01
Equipment: CHAMBER (Hot Air Oven)
Model: UF55 Serial No.: B216.1666
Resolution: 0.1 °C ID No.: UAE.WAO.027/2559
Manufacturer: MEMMERT

Date of Calibration: 8 October 2024
Calibration point: 104.0,140.0 and 180.0 °C

Calibration Condition	Temperature (°C)	Relative Humidity (%)	Line Voltage (Volt)
MIN	29.3	54	227.0
MAX	31.2	56	232.0

Table 1 : Reporting of Temperature

Calibration point (°C)	Measured Temperature (°C) @ Sensor No. (Sensor No.9 is REF)									Uncertainty ± (°C)
	# 1	# 2	# 3	# 4	# 5	# 6	# 7	# 8	# 9	
104.0	103.89	103.66	103.88	103.89	104.40	103.98	103.70	104.10	104.15	0.53
140.0	139.85	139.53	139.87	139.88	140.67	140.00	139.60	140.25	140.23	0.73
180.0	179.63	179.22	179.71	179.76	181.03	180.06	179.41	180.87	180.39	0.90

Table 2 : Reporting of Characterization Result

UUC* Setting (°C)	UUC* Reading (°C)			Stability ± (°C)	Uniformity (°C)	Overall Variation (°C)
	MIN	MAX	Average			
104.0	104.0	104.0	104.0	0.15	0.49	0.88
140.0	140.0	140.0	140.0	0.13	0.71	1.2
180.0	180.0	180.0	180.0	0.13	1.2	1.9

Note: The quoted uncertainty include " Stability " and " Loading effect (20% of Temp Uniformity) " * UUC* = Unit Under Calibration

Stability = One-half of the greatest maximum difference of measured temperatures at any one sensors, for at least half an hour after reaching steady state.

Uniformity = The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time.

Overall Variation = The difference of the maximum and minimum measured temperatures throughout observation time.

The report uncertainty of measurement was based on standard uncertainty multiplied by coverage factor k= 2, providing a level of confidence of approximately 95 %.

***** End *****

F-C5-012 Revision: 01 Date: 20-04-65

เอกสารไม่ควบคุม เอกสารไม่ควบคุม

DQE Services Co.,Ltd.
32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Bangkok 10230
Phone : +66 (0)2 538 2054, Email : dqeservicesinfo@gmail.com

CERTIFICATE OF CALIBRATION

Certificate No. : SP24-018
Customer : United Analyst and Engineering Consultant Co.,Ltd. (Head Office)
Address : 3 Soi Udomsuk 41, Sukhumvit Road, Bangchack, Phrakhanong, Bangkok 10260
Location of calibration : Laboratory 315
Equipment : UV-Vis Spectrophotometer
Manufacturer : Agilent Technologies
Model : Cary 60
Serial No. : MY15410009
ID No. : UAE.WAT.020/2558
Received Date : 7 May 2024
Calibration Date : 7 May 2024
Issue Date : 9 May 2024
Condition Instrument : Good

Calibrated by : (Mr.Tanawat Rittidach)
Approved by : (Ms.Chonchicha Sangngern)
Quality Manager

The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only.

The measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the price written approval of the DQE Services Co., Ltd.

DQE Services Co.,Ltd.

DQE Services

32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Bangkok 10230

Phone : +66 (0)2 538 2054, Email : dqeservicesinfo@gmail.com

MSC-TS169 17025
CALIBRATION DATA

REPORT OF CALIBRATION

Certificate No. : SP24-018

Page 2 of 5

Environment Condition : Ambient Temperature 25 ± 5 °C

Relative humidity 55 ± 20 %RH

Calibration method : In-house method CP-01 Based on ASTM E275-08

Certified Reference Materials :

Material	Serial No.	Certificate No.	Due date
Absorbance Standard set	25760	115663	25 October 2025
Absorbance Standard set	25757	115638	25 October 2025
Wavelength Standard set	25806	115657	25 October 2025
Wavelength Standard set	25758	115665	25 October 2025

Traceability : This certification is traceable to the International System of Unit maintained at National -
Institute of Standards and Technology (NIST) through Starna Scientific Limited

Spectral Band Width of UUC : 1.5 nm.

Scan Speed of UUC : 60 nm/min

Scan Interval of UUC : 0.15 nm.

Resolution of UUC : Photometric 0.0001 Abs.

Wavelength 0.1 nm.

เอกสารไม่ควบคุม

DQE Services Co.,Ltd.

DQE Services

32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Bangkok 10230

Phone : +66 (0)2 538 2054, Email : dqeservicesinfo@gmail.com

MSC-TS169 17025
CALIBRATION DATA

REPORT OF CALIBRATION

Certificate No. : SP24-018

Page 3 of 5

Calibration Results : Without adjustment

Photometric Accuracy :

Wavelength (nm.)	CRMs Values (Abs)	UUC Reading (Abs)	Correction (Abs)	Uncertainty (Abs)	Coverage factor k
420	0.0000	0.0000	0.0000	0.0028	2.00
	0.5780	0.5747	0.0033	0.0031	2.00
	1.0484	1.0438	0.0046	0.0029	2.00
	2.1876	2.1832	0.0044	0.0080	2.00
440	0.0000	0.0000	0.0000	0.0028	2.00
	0.5595	0.5581	0.0014	0.0034	2.00
	1.0239	1.0231	0.0008	0.0035	2.00
	2.1230	2.1219	0.0011	0.0080	2.00
465	0.0000	0.0000	0.0000	0.0028	2.00
	0.5230	0.5184	0.0046	0.0030	2.00
	0.9633	0.9614	0.0019	0.0029	2.00
	1.9753	1.9731	0.0022	0.0070	2.00
546.1	0.0000	0.0000	0.0000	0.0028	2.00
	0.5181	0.5150	0.0031	0.0031	2.00
	1.0002	0.9964	0.0038	0.0033	2.00
	1.9973	1.9914	0.0059	0.0088	2.00
590	0.0000	0.0000	0.0000	0.0028	2.00
	0.5517	0.5485	0.0032	0.0030	2.00
	1.0803	1.0772	0.0031	0.0030	2.00
	2.0373	2.0293	0.0080	0.0080	2.00
635	0.0000	0.0000	0.0000	0.0028	2.00
	0.5591	0.5565	0.0026	0.0031	2.00
	1.0518	1.0482	0.0036	0.0030	2.00
	1.9274	1.9202	0.0072	0.0079	2.00

เอกสารไม่ควบคุม

DQE Services Co.,Ltd.

DQE Services

32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Bangkok 10230

Phone : +66 (0)2 538 2054, Email : dqeservicesinfo@gmail.com

MSC-TS169 17025
CALIBRATION DATA

REPORT OF CALIBRATION

Certificate No. : SP24-018

Page 4 of 5

Photometric Accuracy :

Wavelength (nm.)	CRMs Values (Abs)	UUC Reading (Abs)	Correction (Abs)	Uncertainty (Abs)	Coverage factor k
235	0.0000	0.0000	0.0000	0.0050	2.00
	0.7469	0.7435	0.0034	0.0057	2.00
257	0.0000	0.0000	0.0000	0.0050	2.00
	0.8674	0.8639	0.0035	0.0060	2.00
313	0.0000	0.0000	0.0000	0.0050	2.00
	0.2919	0.2907	0.0012	0.0051	2.00
350	0.0000	0.0000	0.0000	0.0050	2.00
	0.6430	0.6402	0.0028	0.0055	2.00

เอกสารไม่ควบคุม

DQE Services Co.,Ltd.

DQE Services

32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Bangkok 10230

Phone : +66 (0)2 538 2054, Email : dqeservicesinfo@gmail.com

MSC-TS169 17025
CALIBRATION DATA

REPORT OF CALIBRATION

Certificate No. : SP24-018

Page 5 of 5

Wavelength Accuracy :

CRMs Values (nm.)	UUC Reading (nm.)	Correction (nm.)	Uncertainty (nm.)	Coverage factor k
241.72	242.0	-0.28	0.18	2.00
279.45	279.5	-0.05	0.18	2.00
287.81	287.9	-0.09	0.18	2.00
334.06	333.9	0.16	0.18	2.00
360.93	360.5	0.43	0.18	2.00
418.59	418.1	0.49	0.18	2.00
445.94	445.6	0.34	0.18	2.00
453.66	453.3	0.36	0.18	2.00
460.02	459.8	0.22	0.18	2.00
536.59	536.0	0.59	0.18	2.00
637.98	638.7	-0.72	0.18	2.00
431.38	430.8	0.58	0.18	2.00
472.50	472.4	0.10	0.18	2.00
513.47	513.7	-0.23	0.18	2.00
528.88	529.1	-0.22	0.18	2.00
573.17	573.5	-0.33	0.18	2.00
585.35	585.2	0.15	0.20	2.00
684.40	685.1	-0.70	0.18	2.00
740.72	741.4	-0.68	0.20	2.00
748.55	749.1	-0.55	0.18	2.00
807.03	807.3	-0.27	0.18	2.00
879.28	879.3	-0.02	0.18	2.00

Remark : - UUC = Unit Under Calibration

- N/A = Not Available

- The result expanded uncertainty of measurement U is stated as the standard uncertainty of measurement multiplied by the coverage factor k,

which for a normal distribution corresponds to a coverage probability of approximately 95%

- * Indicates non TISI accredited

- End of Certificate -

เอกสารไม่ควบคุม

DQE Services Co.,Ltd.

DQE Services

32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Bangkok 10230

Phone : +66 (0)2 538 2054, Email : dqeservicesinfo@gmail.com

ISO 17025

LABORATORY DATA

CERTIFICATE OF CALIBRATION

Certificate No. : SP24-028

Page 1 of 5

Customer : United Analyst and Engineering Consultant Co.,Ltd. (Head Office)

Address : 3 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260

Location of calibration : Laboratory 315

Equipment : UV-Vis Spectrophotometer

Manufacturer : HITACHI

Model : U-5100

Serial No. : 23A4-008

ID No. : UAE.WAS.010/2567

Received Date : 10 September 2024

Calibration Date : 10 September 2024

Issue Date : 13 September 2024

Condition Instrument : Good

Calibrated by :

(Mr.Tanawut Rittidach)

Technical Manager

Approved by :

(Ms.Chonthicha Sangngern)

Quality Manager

The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only.

The measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the DQE Services Co., Ltd.

เอกสารไม่ควบคุม

FM-708-02 R01 1/1/2021

DQE Services Co.,Ltd.

DQE Services

32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Bangkok 10230

Phone : +66 (0)2 538 2054, Email : dqeservicesinfo@gmail.com

ISO 17025

LABORATORY DATA

REPORT OF CALIBRATION

Certificate No. : SP24-028

Page 2 of 5

Environment Condition : Ambient Temperature 25 ± 5 °C

Relative humidity 55 ± 20 %RH

Calibration method : In-house method CP-01 Based on ASTM E275-08

Certified Reference Materials :

Material	Serial No.	Certificate No.	Due date
Absorbance Standard set	25760	115663	25 October 2025
Absorbance Standard set	25757	115638	25 October 2025
Wavelength Standard set	25806	115657	25 October 2025
Wavelength Standard set	25758	115665	25 October 2025

Traceability : This certification is traceable to the International System of Unit maintained at National -

Institute of Standards and Technology (NIST) through Stama Scientific Limited

Spectral Band Width of UUC : 5.0 nm.

Scan Speed of UUC : 40

Scan Interval of UUC : 0.1 nm.

Resolution of UUC : Photometric 0.001 Abs.

Wavelength 0.1 nm.

เอกสารไม่ควบคุม

FM-708-02 R01 1/1/2021

DQE Services Co.,Ltd.

DQE Services

32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Bangkok 10230

Phone : +66 (0)2 538 2054, Email : dqeservicesinfo@gmail.com

ISO 17025

LABORATORY DATA

REPORT OF CALIBRATION

Certificate No. : SP24-028

Page 3 of 5

Calibration Results : Without adjustment

Photometric Accuracy :

Wavelength (nm.)	CRMs Values (Abs)	UUC Reading (Abs)	Correction (Abs)	Uncertainty (Abs)	Coverage factor k
420	0.0000	0.000	0.0000	0.0028	2.00
	0.5780	0.575	0.0030	0.0031	2.00
	1.0484	1.044	0.0044	0.0029	2.00
	2.1876	2.190	-0.0024	0.0075	2.00
440	0.0000	0.000	0.0000	0.0028	2.00
	0.5595	0.557	0.0025	0.0034	2.00
	1.0239	1.021	0.0029	0.0035	2.00
	2.1230	2.121	0.0020	0.0079	2.00
465	0.0000	0.000	0.0000	0.0028	2.00
	0.5230	0.519	0.0040	0.0029	2.00
	0.9633	0.961	0.0023	0.0028	2.00
	1.9753	1.975	0.0003	0.0070	2.00
546.1	0.0000	0.000	0.0000	0.0028	2.00
	0.5181	0.515	0.0031	0.0031	2.00
	1.0002	0.997	0.0032	0.0033	2.00
	1.9973	1.996	0.0013	0.0085	2.00
590	0.0000	0.000	0.0000	0.0028	2.00
	0.5517	0.549	0.0027	0.0030	2.00
	1.0803	1.078	0.0023	0.0029	2.00
	2.0373	2.031	0.0063	0.0081	2.00
635	0.0000	0.000	0.0000	0.0028	2.00
	0.5591	0.557	0.0021	0.0031	2.00
	1.0518	1.049	0.0028	0.0029	2.00
	1.9274	1.923	0.0044	0.0080	2.00

เอกสารไม่ควบคุม

FM-708-02 R01 1/1/2021

DQE Services Co.,Ltd.

DQE Services

32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Bangkok 10230

Phone : +66 (0)2 538 2054, Email : dqeservicesinfo@gmail.com

ISO 17025

LABORATORY DATA

REPORT OF CALIBRATION

Certificate No. : SP24-028

Page 4 of 5

Photometric Accuracy :

Wavelength (nm.)	CRMs Values (Abs)	UUC Reading (Abs)	Correction (Abs)	Uncertainty (Abs)	Coverage factor k
235	0.0000	0.000	0.0000	0.0050	2.00
	0.7469	0.743	0.0039	0.0056	2.00
257	0.0000	0.000	0.0000	0.0050	2.00
	0.8674	0.862	0.0054	0.0059	2.00
313	0.0000	0.000	0.0000	0.0050	2.00
	0.2919	0.291	0.0009	0.0051	2.00
350	0.0000	0.000	0.0000	0.0050	2.00
	0.6430	0.639	0.0040	0.0055	2.00


เอกสารไม่ควบคุม

FM-708-02 R01 1/1/2021

DQE

Services

32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Bangkok 10230
Phone : +66 (0)2 538 2054, Email : dqeservicesinfo@gmail.com



DQE
ISO 15189:2013
CALIBRATION 0404

REPORT OF CALIBRATION

Certificate No. : SP24-028

Page 5 of 5

Wavelength Accuracy :

CRMs Values	UUC Reading	Correction	Uncertainty	Coverage factor
(nm.)	(nm.)	(nm.)	(nm.)	k
241.00	240.4	0.60	0.18	2.00
279.30	278.7	0.60	0.18	2.00
288.90	288.5	0.40	0.18	2.00
334.50	334.2	0.30	0.18	2.00
361.40	361.1	0.30	0.18	2.00
418.40	418.0	0.40	0.18	2.00
447.20	446.7	0.50	0.18	2.00
459.30	459.6	-0.30	0.18	2.00
537.00	536.6	0.40	0.18	2.00
638.00	637.4	0.60	0.18	2.00
441.29	440.8	0.49	0.18	2.00
479.88	479.6	0.28	0.18	2.00
513.75	513.5	0.25	0.18	2.00
528.59	528.6	-0.01	0.18	2.00
575.10	574.9	0.20	0.18	2.00
585.56	585.3	0.26	0.20	2.00
684.70	684.1	0.60	0.18	2.00
740.51	740.0	0.51	0.20	2.00
747.61	747.2	0.41	0.18	2.00
807.04	806.3	0.74	0.18	2.00
879.68	878.9	0.78	0.18	2.00

Remark : - UUC = Unit Under Calibration

- N/A = Not Available

- The result expanded uncertainty of measurement U is stated as the standard uncertainty of measurement multiplied by the coverage factor k.

which for a normal distribution corresponds to a coverage probability of approximately 95%

- End of Certificate -

เอกสารไม่ควบคุม
FM-708-02 R01 1/11/2021



Certificate of Calibration

Equipment: CONDUCTIVITY METER
Model: SevenDirect SD30
Serial No. (or ID.): C441872132 (UAE.WAO.017/2567)
Manufacturer: METTLER TOLEDO
Electrode Serial No. 5824370998
Condition: In Condition

Certificate No.: C24250010
Issued Date: 15 January 2025
Job No.: WO-00057642
Page: 1 of 2
Model: InLab 731-ISM
Brand: METTLER TOLEDO

Customer: United Analyst and Engineering Consultant Co., Ltd.
 3 Soi Udomsuk 41, Sukhumvit Road, Bangchak Sub-District,
 Phrakhanong District, Bangkok, THAILAND 10260

Environment Condition: Temperature 21.7 °C ± 0.2 °C
 Humidity 48.8 %RH ± 2.1 %RH

Calibration Place: United Analyst and Engineering Consultant Co., Ltd. (Calibration Laboratory)
 3 Soi Udomsuk 41, Sukhumvit Road, Bangchak Sub-District,
 Phrakhanong District, Bangkok, THAILAND 10260

Calibration By: Mr.Atachai Ngamchanat

Calibration Date: 15 January 2025

The Method used: In house method, CAL-WI-49, base on ASTM D 1125-14 and D 5391-14

Traceability: This certificate is traceable to the SI Units maintained by CRM of NIST(SRM) through CPA chem Co., Ltd. (ISO/IEC 17034) Certificate No. 1066606, 1066608, 1066610

(Mr. Atachai Ngamchanat)

Person in charge

(Miss Kaewkan Suradech)

Authorized signatory

This certificate is issued the units of measurement according to the International System of Units (SI). It provides traceability of measurement to international or national standard or other recognized national standard laboratories.

The measurement uncertainty stated is the expanded uncertainty which is obtained from the standard uncertainty multiplied by the coverage factor (k=2) to provide a level of confidence of approximately 95%. It is determined in accordance with the Guide to Expression of Uncertainty in Measurement (GUM).

These results may be affected by deviations from specified conditions. The results relate only to the items tested, calibrated or sampled. The report shall not be reproduced except in full without approval of DKSH Technology Limited.

บริษัท ดีเคเอส อีเซีย จำกัด
 DKSH Technology Limited
 2533 ถนนสุขุมวิท แขวงคลองเตย เขตคลองเตย กรุงเทพมหานคร 10260
 2533 Sukhumvit Road, Bangkok, Phrakhanong, Bangkok 10260
 Phone : +66 2639 7000 Email : info.calibration@dksh.com Website : www.dksh.com/scientific-thailand

Delivering Growth – in Asia and Beyond.

เอกสารไม่ควบคุม
CAL-FM-C24-09: 12 Sep 2022



Certificate No.: C24250010

Page: 2 of 2

Calibration Results:

Before Adjustment

Standard	Unit Under Calibration	Correction	Coverage Factor	Uncertainty (±)
Conductivity Solution	Reading		(k)	
25.000 µS/cm	24.8 µS/cm	0.200 µS/cm	2.00	0.28 µS/cm
1413.1 µS/cm	1398.4 µS/cm	14.7 µS/cm	2.00	11 µS/cm
111.3 mS/cm	109.5 mS/cm	1.8 mS/cm	2.00	0.81 mS/cm

After Adjustment ; at 1413.1 µS/cm

Standard	Unit Under Calibration	Correction	Coverage Factor	Uncertainty (±)
Conductivity Solution	Reading		(k)	
25.000 µS/cm	25.1 µS/cm	-0.100 µS/cm	2.00	0.28 µS/cm
1413.1 µS/cm	1413.1 µS/cm	0.0 µS/cm	2.00	11 µS/cm
111.3 mS/cm	110.2 mS/cm	1.1 mS/cm	2.00	0.81 mS/cm

The End of Certificate



Refer to Certificate No.: C24250010

Page: 1 of 3

Statements of conformity:

This conformity certificate documents the validity of the following statements of conformity based on the measurement results of corresponding calibration certificate:

The error of temperature determined during calibration are under given measurement and environmental conditions and considering the expanded measurement uncertainty (coverage probability 95%) within the specification. The given measurement uncertainty already includes other all effects by according to the standard method, ASTM D 1125-14 and D 5391-14. Therefore, those parameters have not been assessed separately.

Tolerance and Decision rules:

Assessment of the conformity of the measurement device are done based on direct comparison of the relevant measurement results with the tolerances and decision rule are prescribed by the customer.

- Decision rule :**
- ☐ Choice A Binary Statement for Simple Acceptance Rule (w = 0), Specific Risk < 50% PFA
 - ☒ Choice B Non-binary statement with guard band (w = 1 U), Pass or Fail Specific Risk < 2.5% PFA and Condition Pass or Condition Fail Specific Risk < 50% PFA.
 - ☐ Choice C Customer defined, Customers may define arbitrary multiple of r to have applied as guard band (w = r U).
- ; PFA – Probability of False Accept

(Miss Kaewkan Suradech)

Authorized signatory


Statements of conformity

Before Adjustment

Unit	Conductivity Solution		Correction	Guard band (w)	Tolerance (±)	Conformity
	Standard	UUC				
µS/cm	25.000	24.8	0.200	0.28	1.25	Pass
µS/cm	1413.1	1398.4	14.7	11	70.7	Pass
mS/cm	111.3	109.5	1.8	0.81	5.6	Pass

The validity of the statements of conformity cannot be guaranteed for different places of use, environmental conditions or improper use.

Before Adjustment

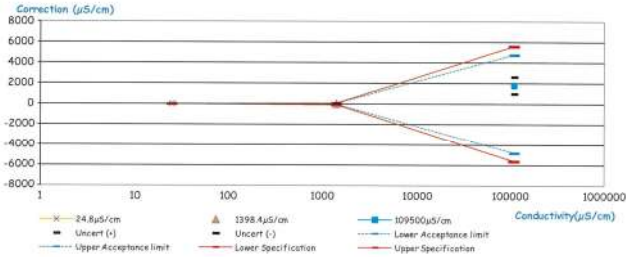

บริษัท ดีเคเอส อีซี จำกัด
DKSH Technology Limited
2533 ถนนสุขุมวิท แขวงคลองเตย เขตคลองเตย กรุงเทพมหานคร 10260
Phone: +66 2639 7000 Email: info.calibration@dksh.com Website: www.dksh.com/scientific-thailand

Delivering Growth - in Asia and Beyond.

เอกสารไม่ควบคุม

CAL-FM-C24-05: 12 Sep 2022


Statements of conformity (cont.)

After Adjustment ; at 1413.1 µS/cm

Unit	Conductivity Solution		Correction	Guard band (w)	Tolerance (±)	Conformity
	Standard	UUC				
µS/cm	25.000	25.1	-0.100	0.28	1.25	Pass
µS/cm	1413.1	1413.1	0.0	11	70.7	Pass
mS/cm	111.3	110.2	1.1	0.81	5.6	Pass

The validity of the statements of conformity cannot be guaranteed for different places of use, environmental conditions or improper use.

After Adjustment ; at 1413.1 µS/cm

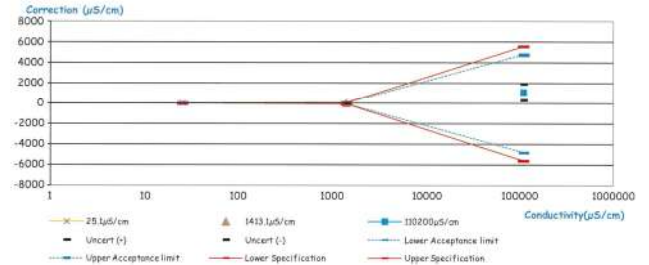

บริษัท ดีเคเอส อีซี จำกัด
DKSH Technology Limited
2533 ถนนสุขุมวิท แขวงคลองเตย เขตคลองเตย กรุงเทพมหานคร 10260
Phone: +66 2639 7000 Email: info.calibration@dksh.com Website: www.dksh.com/scientific-thailand

Delivering Growth - in Asia and Beyond.

เอกสารไม่ควบคุม

CAL-FM-C24-05: 12 Sep 2022

ใบตรวจสอบสภาพเครื่องวัดสิ่งแวดล้อม

เลขที่ใบงาน: WO-00057642

ชนิดเครื่องมือ: CONDUCTIVITY METER

รุ่น: SevenDirect SD30

หมายเลขเครื่อง: C441872132

ตรวจสอบ (รับ)		รายการตรวจเช็ค	ตรวจสอบ (ส่ง)		หมายเหตุ
15 Jan 2025			15 Jan 2025		
ปกติ	ไม่ปกติ		ปกติ	ไม่ปกติ	
		General			
<input checked="" type="checkbox"/>	<input type="checkbox"/>	1. ความสมบูรณ์เครื่อง	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	2. ความสะอาด (ช่องใส่ตัวอย่าง, ภายใน-นอกเครื่อง)	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	3. สวิตช์ ปิด - เปิด เครื่อง (On-Off Switch)	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	4. ปุ่มกด (Keypad)	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	5. หน้าจอ (Display, Screen Contrast)	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
		Spectrophotometer			
<input type="checkbox"/>	<input type="checkbox"/>	6. แบตเตอรี่ไฟฟ้า (Battery Backup) >= 2.5 VDC	<input type="checkbox"/>	<input type="checkbox"/>	
<input type="checkbox"/>	<input type="checkbox"/>	7. ตัวควบคุมเลือกความยาวคลื่น (Wavelength Control)	<input type="checkbox"/>	<input type="checkbox"/>	
<input type="checkbox"/>	<input type="checkbox"/>	8. ความยาวคลื่น (Wavelength Check)	<input type="checkbox"/>	<input type="checkbox"/>	
<input type="checkbox"/>	<input type="checkbox"/>	9. แหล่งกำเนิดแสง (UV < 3,000 hour)	<input type="checkbox"/>	<input type="checkbox"/>	
<input type="checkbox"/>	<input type="checkbox"/>	10. แหล่งกำเนิดแสง (Visible < 5,000 hour)	<input type="checkbox"/>	<input type="checkbox"/>	
<input type="checkbox"/>	<input type="checkbox"/>	11. ช่องจัดหลายตัวอย่าง (Carousel Module)	<input type="checkbox"/>	<input type="checkbox"/>	
		pH Meter and Conductivity Meter			
<input checked="" type="checkbox"/>	<input type="checkbox"/>	12. อิเล็กโทรด (Electrode and Connection Cable)	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input type="checkbox"/>	<input type="checkbox"/>	13. ระดับสารละลายใน Electrode (Level KCl)	<input type="checkbox"/>	<input type="checkbox"/>	
<input type="checkbox"/>	<input type="checkbox"/>	14. ฝาปิดกันละออง Electrode (Dust Protection Hood)	<input type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	15. ขาจับอิเล็กโทรด (Stand)	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
		Turbidimeter			
<input type="checkbox"/>	<input type="checkbox"/>	16. ค่าความขุ่นต่ำสุด (No Sample)	<input type="checkbox"/>	<input type="checkbox"/>	
<input type="checkbox"/>	<input type="checkbox"/>	17. ระดับการส่องสว่างของแสง (>= 2.5 ไม่น้อย 3.0)	<input type="checkbox"/>	<input type="checkbox"/>	
		Automatic titrator			
<input type="checkbox"/>	<input type="checkbox"/>	18. สภาพ Piston Burettes	<input type="checkbox"/>	<input type="checkbox"/>	
<input type="checkbox"/>	<input type="checkbox"/>	19. Function Rinsing and Dosing	<input type="checkbox"/>	<input type="checkbox"/>	
<input type="checkbox"/>	<input type="checkbox"/>	20. ระบบท่อสายยางและอุปกรณ์ประกอบ	<input type="checkbox"/>	<input type="checkbox"/>	

*ข้อแนะนำ : Electrode วัดอุณหภูมิได้ 25.1°C โดย Control Waterbath ที่ 25.0 ± 0.5°C

Mr.Atachai Ngamchanat

Service Engineer

เอกสารไม่ควบคุม

CAL-FM-R31-03: 20 Jul 2022

บริษัท ดีเคเอส อีซี จำกัด
DKSH Technology Limited
2533 ถนนสุขุมวิท แขวงคลองเตย เขตคลองเตย กรุงเทพมหานคร 10260
Phone: +66 2639 7000 Email: info.calibration@dksh.com Website: www.dksh.com/scientific-thailand

Delivering Growth - in Asia and Beyond.



Certificate of Calibration

Cert. No.: 24TM1114
Page : 1 of 3

Equipment :	BOD Incubator
Manufacturer :	ARCO
Model :	UC4-1320
Serial No. :	-
ID No. :	UAE.WAO.018/2559
Submitted by :	United Analyst and Engineering Consultant Co.,Ltd. 3 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Location :	Lab Floor 2
Received Order :	11 July 2024
Calibration Date :	11 July 2024
Ambient Temperature :	(26 ± 10) °C
Relative Humidity :	(50 ± 30) %
Calibrated by :	Tawatchai Pama
Approved by :	
	Approved Signatory
	() Ponpan Paipim
	(✓) Suwit Imjai
	() Kunchit Promprat
Issue Date :	14 July 2024

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written Approval of the head of Corporate Services 3: Equipment Calibration and Testing Services.

เอกสารไม่ควบคุม



Equipment : BOD Incubator
Condition As-Received : Used Item
Reference : 2407-0243OC-2
Procedure Used :-

Cert. No.: 24TM1114
Page : 2 of 3

Calibration were conducted using calibration procedure CP-OT02 based on TLAS G-20 according to direct measurement method with Data Acquisition which connected with Resistance Temperature Detector (RTD).
The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

Instrument	Serial No.	Cert. No.	Traceable	Due Date
1) Data Acquisition	MY49023932	23LM122	TPA	26 Jul 2024


2. This certificate is valid only to the item calibrated on date and place of calibration.
3. This certification is traceable to the International System of Unit.

Remark : TPA : Technology Promotion Association (Thailand - Japan)

Result of Calibration :- (*) Without Adjustment

Function of UUC* : Temperature Source

Fresh air setting : Not Available



Probe Installation Details :

a = 10 cm
b = 10 cm
c = 10 cm

Dimension of Chamber :

D = 0.62 m
W = 1.2 m
H = 1.2 m
Capacity = 0.89 m³

Environment during calibration		
	Beginning	Finished
Temp. (°C)	29	29
REL.Humid. (%)	78	72
AC Supply (Volt)	233	234

Position :	Ref. Std. ID No.:
1	20-16RTD-10
2	20-16RTD-02
3	20-16RTD-03
4	23-16RTD-04
5	22-16RTD-05
6	20-16RTD-06
7	20-16RTD-07
8	22-16RTD-08
9 (ref.)	22-16RTD-09



Equipment : BOD Incubator
Condition As-Received : Used Item
Reference : 2407-0243OC-2
Result of Calibration :- (*) Without Adjustment
Function of UUC* : Temperature Source
Fresh air setting : Not Available

Cert. No.: 24TM1114
Page : 3 of 3

Calibration Point (°C)	UUC* Setting (°C)	UUC* Reading (°C)	Temperature stability (± °C)	Temperature uniformity (°C)	Overall Variation (°C)	Coverage Factor k
20.0	20.0	19.9	0.29	0.81	1.2	2

Calibration Point (°C)	Measured Temperature (°C)									Uncertainty (± °C)
	1	2	3	4	5	6	7	8	9 (ref.)	
20.0	20.361	19.640	20.312	20.079	19.908	19.872	19.955	19.818	19.758	0.48

Average* : The average of 30 values in each position.

Temperature stability : One-half of the greatest maximum difference of measured temperature at any one sensor.

Temperature uniformity : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.

Overall Variation : The Difference of the maximum and minimum measured temperatures throughout observation.

UUC* : Unit Under Calibration

Note : The reported uncertainty of measurement was included stability and excluded uniformity .

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k, providing a level of confidence of approximately 95 %.

-000-

เอกสารไม่ควบคุม

เอกสารไม่ควบคุม



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3 : EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL: 0-2717-3000 FAX: 0-2719-9484

Certificate of Testing

Cert.No.: 24TW222
Page.: 1 of 2

Equipment : DO Meter
Manufacturer : YSI
Model : 4010-2W
Serial No. : 20260326
ID No. : UAE.WAO.060/2563
Received Date : 16 October 2024
Test Date : 17 October 2024
Reference : 2410-0532DSC-1
Submitted by : United Analyst and Engineering Consultant Co.,Ltd.
3 Sol Udomsuk 41, Sukhumvit Road, Bangchak, Pitrakhanong, Bangkok 10260
Laboratory Condition : Temperature (25 ± 5) °C
Humidity (50 ± 20) %
Test Procedure : In - house method : CP-CH9
by Comparison Technique with Azide Modification Method

Tested by : Walalak Sirthean

Approved by :

Saithip
Approved Signatory

() Unnophol Harachai
() Ponpan Palpim
(✓) Saithip Meangmai

Issue Date : 17 October 2024



Cert.No.: 24TW222
Page.: 2 of 2

Condition of this result of calibration

1. Reference Standard Instruments :

This certification is traceable to the International System of Unit through the reference standards laboratory of Industrial Calibration Center, Technology Promotion Association (Thailand-Japan).

Instruments	Serial No.	ID No.	Certificate No.	Due Date
1. Burette	-	130BU10	23CG1172	22 Mar 2025
2. Balance	14233821	110RC001	24MM131	04 July 2025

2. Standard Material :-

Material	Manufacturer	Lot.No.	Assay
Sodium Thiosulfate 5-Hydrate AR	KEMAUS	2203162447	99.6%

Result : Dissolved Oxygen Meter Adjustment With Air 100 %
Dissolved Oxygen Probe No.: 22M102385

Titration Method (Azide Modification Method)	DO Meter Reading (mg/L)	Standard Deviation (mg/L)
8.18	8.24	0.0071

This report was certified only for the instrument we tested. It is allowable to use for study intend to use for advertising and referral purpose is prohibited. This report may not be reproduced other in full, without written approval of the laboratory

-000-

เอกสารไม่ควบคุม

เอกสารไม่ควบคุม


Certificate No. : HIT-2417-0568

Page : 1 of 2

CERTIFICATE OF CALIBRATION

Equipment : COD Test Tube Heater
Meter Model : HI839800-02 Serial No. : 1147807
Tube Heater : 25 Vial Capacity Resolution : 0.1°C
Temperature Range : (-10 to 160)°C Temperature of Reaction : 150°C
Manufacturer : Hanna Instruments Made in : Romania
Condition As-Received : Used Product Reference : RE240681
Ambient Temperature : (25 ± 2)°C Relative Humidity : (50 ± 15)%RH
Customer name : United Analyst and Engineering Consultant Co., Ltd.
3 Soi Udomsuk 41, Sukhumvit Rd., Bangchak,
Phrakhanong, Bangkok 10260
Received date : 22 April 2024
Calibrate date : 23 April 2024
Issue date : 25 April 2024
Calibrated Location : Hanna Instruments (Thailand) Ltd.
Calibration Procedure : This calibrator was conducted by using in-house: calibration procedure
CP-04 by using certified reference standard instruments.

Calibrated by : ☒ Mr. Pichit Petthong
☐ Mr. Channarong Soinak

Approved by : 
Mr. Anan Suwanchaisakul
Authorized Signatory



This certificate was certified only for the instrument we calibrated.

This result of calibration was found accurate on date and place of calibration only.

** This certificate may not be reproduced other than in full, except with the prior written **

approval of the head of Hanna Instrument (Thailand).

เอกสารไม่ควบคุม

Condition of this calibration result:

Reference Standard Instruments : This certification is traceable to the international unit of unit maintained through:

Instruments	Model	Serial No.	Certificate No.	Traceable
Data Acquisition Switch Unit	34970A	MY44065265	WK2307-164-1	WK Electric Co., Ltd.
Digital Thermo-Hygrometer	HT-771SD	AL07155	24H41	Technology Promotion Association (Thailand-Japan).

Calibration Result:

Measurement Temperature Source Accuracy for COD Reactor.

Capacity (Vial)	Nominal Value (°C)	Average Value (°C)	Uncertainty of Measurement (±°C)
25 Vial	150.0	149.8	0.49

Unit : °C

(1A)	(2A)	(3A)	(4A)	(5A)
148.901	149.249	149.950	150.042	149.186
(1B)	(2B)	(3B)	(4B)	(5B)
149.724	149.578	149.852	150.100	150.117
(1C)	(2C)	(3C)	(4C)	(5C)
149.863	149.799	150.233	149.847	149.977
(1D)	(2D)	(3D)	(4D)	(5D)
149.550	149.666	149.958	149.744	149.819
(1E)	(2E)	(3E)	(4E)	(5E)
150.044	149.869	149.361	149.973	149.654

Figure: Shows the location of the temperature source.

The report uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%.

** End of certificate **

เอกสารไม่ควบคุม

PinAAcle 900F
Preventive Maintenance Report

PinAAcle 900F Preventive Maintenance (PM)

Company Name:	V g F 3 3 ๙๖๗ s
Address (Instrument Location):	S1 N l ๙ 5 nr 1u4hu
Serial Number:	(er M4uuR1mu4
PM Number:	4 4
Customer Name (if applicable):	5s
Telephone Number:	untadddku5m
Customer Support Engineer Name:	5s3
Service Order Number:	/ Wu4i ki dnu
Date PM Performed: (DD-MMM-YYYY)	14-May-2024
Next PM Due Date: (DD-MMM-YYYY)	14-Nov-2024
Standard Labor Hours to Complete PM :	5 hours

Part Number	Release	Publication Date	
09370145 Rev.9	A	January 2018	

Scope

The purpose of this PM is to ensure the continued functionality of the PinAAcle 900F by inspecting and replacing any worn or damaged parts. This service should only be performed by a trained representative of PerkinElmer.

The customer should save their method before the PM begins.

General Instructions:

The customer must provide the engineer operational data to demonstrate recent instrument performance prior to starting the PM.

Always check with the customer before making any changes that may affect the customer's analysis or calibration, including a current back-up of system software and/or data files.

The completed document should be signed by an authorized PerkinElmer and customer representative and left with the customer.

Update the PM sticker and instrument logbook as required.

Copyright Information

This document contains proprietary information that is protected by copyright. All rights are reserved.

No part of this publication may be reproduced in any form whatsoever or translated into any language without the prior, written permission of PerkinElmer, Inc.

Copyright © 2013 PerkinElmer, Inc.

Trademarks

Registered names, trademarks, etc. used in this document, even when not specifically marked as such, are protected by law. PerkinElmer is a registered trademark of PerkinElmer, Inc. All other trademarks and registered trademarks not owned by PerkinElmer, Inc. or its subsidiaries that are depicted herein are the property of their respective owners. Except as specifically set forth in its terms and conditions of sale, PerkinElmer makes no Warranty of any kind with regard to this document, including, but not limited to, the implied warranties of merchantability and fitness for a particular purpose.

PerkinElmer shall not be liable for incidental or consequential damages in connection with the furnishing or use of this document.

เอกสารไม่ควบคุม

เอกสารไม่ควบคุม

Company Name: VgF 3 ๙๖๗ s

Instrument Location: S1 N l ๙

(5 nr 1u4hu

Instrument Serial No.: (er M4uuR1mu4

Date: 14-May-2024

Component List

Component / Specific Model	Serial #	Configuration Notes
(gg3 mvue	(er NluuR1nu4	N x Ssusi sl nRid
e 1uuIO f U	1uuN5uSudu1	

Parts Lists

Parts Included with the PM		
Part Number (if applicable)	Description	Quantity
B0501696	Fan Filters	Otg
N3160156	O-Ring Kits for Sampling Introduction (Stainless Steels Nebulizer)	Otg
N3160157	O-Ring Kits for Sampling Introduction (Plastic Nebulizer)	Otg
N9301714	Replacement Acetylene Filter Cartridge	Otg
TH001022	Replacement Air Filter Cartridge	Otg

Additional Reagents and Standards Required for PM				
Part Number (if applicable)	Description	Quality	Batch/Lot #	Expired Date (MM/YY)
N9300183	1000 mg/L Copper Standard	AR	4i dRn3 V 1	Apr 2025

Additional Reagents and Standards Required for PM (Customer Support Solution)				
Part Number (if applicable)	Description	Quantity	Batch/Lot #	Expiration Date (MM/YY)
N/A	DI Water	250 mL	AR	AR
N/A	0.5% HNO ₃	250 mL	AR	AR

เอกสารไม่ควบคุม

Procedure Checklist

Use (✓) to check off those steps in the checklist that have been completed.

1. General:

- ✓ Review the instrument performance with the customer and document any recent problems.
- ✓ Inspect the customer log book and make any appropriate PM entries.
- ✓ Perform general inspection of system for cleanliness.

2. PC Instrument Software:

- ✓ Instrument Software user files/databases archived, packed, and/or deleted as needed.

3. Mechanical:

- ✓ Inspect and clean all fans and filters. Replace filters if necessary
- ✓ Inspect all gas lines for leaks and/or wear. Replace if needed.
- ✓ Clean exterior of the instrument.
- ✓ Inspect the burner head, burner chamber, and nebulizer. Clean if needed as stated in the Hardware Guide.
- ✓ Check burner head dimensions with the feeler gauge as stated in the Hardware Guide in the Maintenance chapter section on cleaning the burner head and checking sloth width. Replace if out of specification
- ✓ Check the condition of the end cap, burner head, and nebulizer O-rings. Replace if necessary.
- ✓ Check the drain system for signs of wear. Replace worn or damaged parts.
- ✓ Visually check for proper flame conditions when igniting the Air-C2H2 and N2O-C2H2 flames (if applicable).

4. Electrical:

- ✓ Inspect PC boards. Clean if necessary.
- ✓ Carefully check all internal and external cable connections.
- ✓ Check instrument firmware revisions upgrade to current levels (if necessary)
- ✓ Run Diagnostics Test within the Advanced function of the Spectrometer page. Check the results in the service log folder in the Spectrometer BM Log Viewer.

5. Optics:

- ✓ Inspect and clean the sample compartment windows, if needed.
- ✓ Inspect optics. Clean or replace if necessary,

6. Gasses:

- ✓ Verify that the Gasses supplied to the instrument are within the pressure and purity specifications found in the PinAAcle 900 Series Pre-installation Checklist SDB.
- ✓ Verify that the acetylene filter and air filter element is dry. Replace if necessary.

เอกสารไม่ควบคุม

Additional Tools Required for PM

Part Number (if applicable)	Description	Quantity	Serial #
N1013000	0.2A Neutral density filter	1	1u1Ouuknu1d
N1013002	1.0A Neutral density filter	1	1u1Ouuknu1d
03030997	System 2 EDL Driver	1	uRuRumh
N3050605	As System 2 EDL	1	1h15k
N3050121	Cu Lumina HCL	1	uhuS1nnuRu1ku
N3050109	Ba Lumina HCL	1	uh141nnu4uuS1
N3050139	K Lumina HCL	1	uRuK1nnu1u1Ru
N3050152	Ni Lumina HCL	1	ud4i 1nnu4uu4u

เอกสารไม่ควบคุม

7. Flame Interlock Check:

Description: Check to ensure that all safety interlocks are closed.

Parameter	Specification	Test Results	Pass/Fail
Flame Sensor	Air/C ₂ H ₂ Flame correctly shuts down	Active	Passed
Drain Sensor	Air/C ₂ H ₂ Flame correctly shuts down	Active	Passed
Nebulizer Sensor	Air/C ₂ H ₂ Flame correctly shuts down	Active	Passed
C ₂ H ₂ Pressure Sensor	Air/C ₂ H ₂ Flame correctly shuts down	Active	Passed
Air Pressure Sensor	Air/C ₂ H ₂ Flame correctly shuts down	Active	Passed
Burner Head Sensor	Choosing Nitrous Oxide as the oxidant should trigger an interlock shuts down	Active	Passed

8. After PM Performance tests:

8.1 Detector Linearity with Barium

Description: Ensures that the detector is linear in the Visible Range.

Parameter	Specification	Certificate Value at 553.6 nm (Abs.)	Test Results	Pass/Fail
1.0 A ND Filter	± 5% from Cert.	usnmnd	1su1SR	Passed
0.2 A ND Filter	± 5% from Cert.	uslnRih	uslnRih	Passed

8.2 Baseline Noise at 1.0 Absorbance with Barium

Description: Ensures that a high absorbance will not produce excessive noise.

Parameter	Specification	Results	Pass/Fail
Standard Deviation	≤ 0.010	usnu4	Passed

8.3 AA Baseline Noise with Copper

Description: Check baseline noise.

Parameter	Specification	Results	Pass/Fail
Standard Deviation	≤ 0.001	usnuu4	Passed

เอกสารไม่ควบคุม

8.4 D₂ Background Compensation with Copper

Description: Verifies the instruments ability to compensate for Background absorption.

Parameter	Specification	Results	Pass/Fail
Standard Deviation	≤ 0.010	๐.๐๐๑1	Passed

8.5 AA-BG Baseline Noise with Copper

Description: Ensures that background correction does not produce excessive noise.

Parameter	Specification	Results	Pass/Fail
Standard Deviation	≤ 0.005	๐.๐๐๑4	Passed

8.6 AA-BG Baseline Noise with Arsenic

Description: Ensures that background correction does not produce excessive noise at a low wavelength.

Parameter	Specification	Results	Pass/Fail
Standard Deviation	≤ 0.005	๐.๐๐๑4	Passed

8.7 Flame Sensitivity

Description: Instrument Sensitivity checked against Copper standard.

Standard Copper Sensitivity	Specification	Results (Abs.)	Pass/Fail
5 mg/L Sensitivity SS Neb (if applicable)	> 0.250 Abs.	0.๓	Not Applicable
2 mg/L Sensitivity HS Neb (if applicable)	> 0.250 Abs.	๐.๓๐๐๔	Passed



10. Review:

- ☒ Review with the customer PM work performed.
- ☒ Review with the customer routine maintenance procedures.
- ☒ Discuss recommended customer supplied materials to have on hand.
- ☒ Attach PM sticker.

Additional Comments

Additional Comments Regarding the PM

Review

The preventive maintenance checks and if applicable performance tests for PinAAcle 900F have been completed.	
This PinAAcle 900F Passes <input checked="" type="checkbox"/> Fails <input type="checkbox"/> the preventive maintenance.	
Review of Preventive Maintenance:	
Authorized PerkinElmer Representative: 	Date: 14-May-2024 (DD-MMM-YYYY)
Authorized Customer Representative: 	Date: 14-May-2024 (DD-MMM-YYYY)

เอกสารไม่ควบคุม

เอกสารไม่ควบคุม



Agilent CrossLab Start Up Services

Agilent 5100 5110 ICP-OES Preventive Maintenance



Agilent Preventive Maintenance provides factory recommended service for your analytical instruments to assure reliable operation and the accuracy of your results.

Delivered by highly trained and certified service engineers using genuine Agilent parts and supplies, Agilent Preventive Maintenance provides what you need to reduce unplanned downtime and keep your systems operating at their peak performance.

This checklist is used as a guide for completing the preventive maintenance tasks. A signed copy of this checklist is provided for your records.



Introduction

Customer Information

- Customers should provide all necessary operating supplies upon request of the engineer.
- A customer representative should be available to the engineer while performing the preventive maintenance procedures. Customers are responsible for regular maintenance and are encouraged to observe the service representative.
- Any parts not included in the Parts Lists section of this document are not part of the recommended Preventive Maintenance service nor are they included in the price of this service.
- If a system requires the use of extra or special procedures and/or parts for the maintenance service, then these must be ordered separately and charged as a repair, which may incur additional costs.
- For customers using HF applications, the instrument should be returned to its standard sample introduction system.



เอกสารไม่ควบคุม



เอกสารไม่ควบคุม

Important Customer Web Links

- To access **Agilent University**, visit <http://www.agilent.com/crosslab/university/> to learn about training options, which include online, classroom and onsite delivery. A training specialist can work directly with you to help determine your best options.
- To access the **Agilent Resource Center** web page, visit <https://www.agilent.com/en-us/agilentresources>. The following information topics are available:
 - Sample Prep and Containment
 - Chemical Standards
 - Analysis
 - Service and Support
 - Application Workflows
- The **Agilent Community** is an excellent place to get answers, collaborate with others about applications and Agilent products, and find in-depth documents and videos relevant to Agilent technologies. Visit <https://community.agilent.com/welcome>
- Videos about specific preparation requirements for your instrument can be found by searching the **Agilent YouTube** channel at <https://www.youtube.com/user/agilent>
- Need to place a service call? [Flexible Repair Options | Agilent](#)

Service Engineer's Responsibilities

- Contact the customer and ensure that all necessary supplies are available before the preventive maintenance visit.
- Only select those pages that relate to the system or module being serviced.
- Complete empty fields with the relevant information.
- Complete the relevant checkboxes in the checklist using either a "X" or tick mark "✓".
- Check "Service not applicable" check boxes to indicate services/tasks not delivered, as appropriate.
- Complete the Preventive Maintenance services in the most logical order relevant to the individual system service in the order of the tasks listed.
- Complete the **Service Review** section together with the customer.
- Complete the fields for page numbers at the foot of each selected page.
- Add relevant page numbers to selected pages and complete the total number of pages field in the Service Completion section
- Ask the customer to sign the **Service Verification** section including the customer's and your signature.

Instrument Maintenance

System Information

- ☐ Check this box if an instrument configuration report is attached instead of completing the table.

Instrument System Name and ID	5110 VDV ICP-OES
Instrument System Site and Location	United Analyst and Engineering Consultant

List System Component Product Numbers	List the Serial Numbers of each Component
1. G 6015A	MY 19030001
2.	
3.	
4.	
5.	
6.	
7.	
8.	
9.	

ICP-OES Configuration Table	Circle the type or write in the type if other
Nebulizer Type	SeaSpray (OneNeb) Conical Other
Spray Chamber	Cyclonic Single Pass (Cyclonic Double Pass) Other
Torch	Radial (Dual View) Other
Torch Type	One Piece (Semi Demountable) Fully Demountable Other
Injector Diameter	2.4mm (1.8mm) 1.4mm 0.8mm Other
Injector Material	(Quartz) Ceramic Other

Preparation

- ☒ Discuss any specific issues with the customer before starting.
- ☒ Review the instrument logbook for recorded problems and comments.
- ☒ Save instrument control settings before starting the procedure.
- ☒ Perform a general inspection of the system for cleanliness.
- ☒ Check for proper installation of parts, assemblies, sensors etc.
- ☒ Check system for required installation of components and implementation of Service Notes
- ☒ Check for required firmware/software updates and verify with customers if they would like them installed.
- ☐ For HF application systems, if standard sample introduction system was not installed, ask the customer to install it.
- ☒ Ask the customer to remove any samples from the ICP-OES sample introduction area, auto sampler or around the ICP-OES.

Preventive Maintenance Procedures

Record Pre-PM instrument performance

- ☒ Run Instrument Performance test.
- ☒ Record results in Instrument Performance Test Results Table – Pre-PM.

Clean and inspect ICP-OES system

- ☒ Look for any obvious external damage or problems.
- ☒ Inspect water cooling hoses, gas lines and power cord for excessive wear or damage.
- ☒ Perform a general internal inspection of the system for excessive dust accumulation, clean if necessary.
- ☒ Inspect sample introduction components and record any required maintenance in the Service Engineer Comments and notify the customer as the required actions required.
- ☒ Record the instrument operating conditions in the ICP-OES Status Results Table.
- ☒ Replace the polychromator purge filter.
- ☒ Replace the radial pre-optics window.
- ☒ Replace the axial pre-optics window for SVDV and VDV instruments.
- ☒ Check exhaust flow for the correct positive extraction at the exhaust duct to insure they meet minimum specifications.
- ☒ Replace air inlet dust filter.
- ☐ Replace high capacity air inlet dust filter element if installed. ^{N/A}
- ☒ Remove and clean instrument water inlet filter.

Agilent Water Recirculator

- ☐ Service not applicable
- ☒ Drain cooling fluid and remove any particles from the chiller reservoir
- ☒ Remove, clean and reinstall water inlet mesh filter if present.
- ☒ Re fill with Agilent Cool Clear cooling fluid.
- ☒ Clean the cooling system Air filter and the condenser.

SPS 3 Auto Sampler

- ☒ Service not applicable
- ☐ Power cycle the autosampler and verify successful initialization.
- ☐ Inspect X and Z axis belts for wear. Replace is necessary.
- ☐ Clean X and Z axis slide shafts.
- ☐ Using customer's racks and the Agilent software move the sample probe to the 4 outermost corners and rinse port, ensure that the probe is approximately centered in the vial.

SPS 4 Auto sampler

- ☒ Service not applicable
- ☐ Clean the spill tray, rack location mat, end frames and chassis with a damp soft cloth and diluted mild detergent.
- ☐ Clean the auto sampler cover panels, if cover kit is installed, with domestic window cleaner.
- ☐ Check the X-axis and Z-axis drive belts for cracks, splits, damaged teeth, excessive fraying, color changes or degradation from fumes.
- ☐ Check the X-axis, Theta-axis and Z-axis FFC cables for cracks, incorrect positioning, damaged edges or damaged connectors.
- ☐ Pump Tubing Replacement. Replace peristaltic pump tubing. Replace all tubing that goes from the rinse station to the pump and from the pump to the waste/rinse bottles
- ☐ Test using customer's tray and move the sample probe to the sample vial 1, wash vial and rinse port and ensure that the probe is centered in the vial. If not use calibration wizard and calibrate the position.

AVS 4, 6, 7 Advanced Valve System

- ☒ Service not applicable
- ☐ Replace valve rotor seal
- ☐ Check fittings for signs of leaks
- ☐ Check tubing including autosampler tubing for kinks or excessive wear
- ☐ Check high flow pump for signs of leaks

ICP-OES adjustment

- ☒ Check position of Zn peak, adjust if required.
- ☒ Check Argon Ratio, adjust to specified value if required.
- ☒ Perform Detector Calibration.
- ☒ Perform Instrument Calibration.

Record Post-PM instrument performance

- ☒ Run Instrument Performance test.
- ☒ Record results in Instrument Performance Test Results Table - Post PM.
- ☒ For systems using ICP Expert version 7.3 and above, run the following instrument tests
 - ☒ Subsystem Communications Test
 - ☒ Air Flow
 - ☒ Water Flow
 - ☒ Gas Flows
 - ☒ RF Generator
 - ☒ Camera Test
 - ☒ Optics Test
 - ☒ Nebulizer Test
- ☒ Record the result in the Instrument Test Results Table

Restore Instrument

- ☐ For HF applications, ask the customer to reinstall their sample introduction system. ^{N/A}
- ☒ Leave system in an Idle state: on and purging.
- ☒ Guidance: If the PM service is performed prior to a qualification service, then use the qualification procedure as a guide for final instrument set up and checkout.

Service Review

- ☒ Attach available reports/printouts of all tests to this documentation.
- ☒ Record the Preventive Maintenance service activity in the customer's records/logbook.
- ☒ Record the PM event in the Smart Alerts logbook, if applicable.
- ☒ Update/reset instrument maintenance counters as appropriate.
- ☒ Affix the PM sticker to the system or instrument logbook based on the customer's request.
- ☒ Complete the Service Engineer Comments section if there are additional comments.
- ☒ Review this service, parts replaced, and test results obtained with the customer.
- ☒ If the instrument firmware was updated, record the details of the change in the Service Engineer's Comments box. Systems in a compliant environment may need additional documentation.
- ☒ Complete the Signature Page with both Service Engineer and Customer signatures.

Report Summary	
Instrument Model	Agilent 5100/5110 VDV ICP-OES
Instrument ID	G8011A/G8015A
Instrument Serial Number	MY18030001
Software Version	7.3.1.9507
Firmware Version	3442
Tested By	Pre Test_PM_Kanyakorn S.
Test Completed On	11/4/2024 9:19:10 AM
Result Summary	
Subsystem Communications Test	Skipped
Air Flow Test	Skipped
Water Flow Test	Skipped
Gas Flows Test	Skipped
RF Generator Test	Skipped
Camera Test	Skipped
Optics Test	Skipped
Advanced Valve System Test	Skipped
Resolution Test	Pass
Sensitivity Test	Fail
Precision Test	Pass

Page 1 of 4

เอกสารไม่ควบคุม

Resolution Test			Pass
Element Wavelength	Specification	Width	
N (174.213 nm)	≤ 9.40	6.98	
As (188.980 nm)	≤ 8.20	6.17	
C (193.027 nm)	≤ 11.50	8.30	
Mo (202.032 nm)	≤ 8.20	6.38	
Cr (206.158 nm)	≤ 13.40	8.98	
Zn (213.857 nm)	≤ 8.70	6.60	
Pb (220.353 nm)	≤ 9.50	7.09	
Co (228.615 nm)	≤ 17.20	11.67	
Ba (230.424 nm)	≤ 9.40	7.20	
Mn (257.610 nm)	≤ 13.30	9.43	
Mn (260.568 nm)	≤ 20.30	14.11	
Cr (267.716 nm)	≤ 11.00	8.04	
Cu (324.754 nm)	≤ 25.00	18.97	
Cu (327.395 nm)	≤ 14.20	11.23	
Sr (338.071 nm)	≤ 33.50	24.30	
Ba (455.403 nm)	≤ 44.00	33.47	
Sr (460.733 nm)	≤ 36.00	17.23	
Ba (493.408 nm)	≤ 36.00	25.37	
Ba (614.171 nm)	≤ 42.00	25.54	
Ar (675.283 nm)	≤ 74.00	56.51	
K (766.491 nm)	≤ 80.00	65.86	

Page 2 of 4

เอกสารไม่ควบคุม

Sensitivity Test			Fail		
Radial					
Element Wavelength	Specification	Method	Ratio	Standard	Blank
As (188.980 nm)	≥ 46.0	SRBR	104.1	793.0	50.8
Se (196.026 nm)	≥ 41.0	SRBR	87.6	862.0	79.7
Zn (213.857 nm)	≥ 1421.0	SRBR	1500.8	41823.3	749.0
Pb (220.353 nm)	≥ 46.0	SRBR	170.7	2432.0	174.9
Mn (257.610 nm)	≥ 3518.0	SRBR	3915.0	264700.2	4420.0
Al (396.152 nm)	≥ 3.4	SBR	7.7	48454.6	5563.2
Ba (493.408 nm)	≥ 34.0	SBR	45.9	1966719.7	41903.8
K (766.491 nm)	≥ 1.8	SBR	5.7	99038.2	14687.7
Axial					
Element Wavelength	Specification	Method	Ratio	Standard	Blank
As (188.980 nm)	≥ 208.0	SRBR	126.5	1498.8	119.0
Se (196.026 nm)	≥ 159.0	SRBR	112.0	1773.6	197.8
Zn (206.200 nm)	≥ 234.0	SRBR	466.0	6784.2	199.7
Zn (213.857 nm)	≥ 1743.0	SRBR	2217.4	95597.6	1789.7
Cd (214.439 nm)	≥ 4227.0	SRBR	1919.3	68724.6	1236.4
Pb (220.353 nm)	≥ 320.0	SRBR	332.6	7929.5	499.0
Mn (257.610 nm)	≥ 10625.0	SRBR	7492.2	991238.3	16911.7
Cr (267.716 nm)	≥ 1048.0	SRBR	2254.6	129706.6	3150.9
Cu (324.754 nm)	≥ 19.0	SBR	26.9	290746.3	10407.5
Al (396.152 nm)	≥ 6.0	SBR	10.7	211329.2	18005.0
Ba (493.408 nm)	≥ 60.0	SBR	49.3	6956460.4	138336.9
K (766.491 nm)	≥ 24.0	SBR	28.1	1395190.2	47996.2

Page 3 of 4

เอกสารไม่ควบคุม

Precision Test		Pass
Radial		
Element Wavelength	Specification	Measured Value % RSD
As (188.980 nm)	≤ 2.60	0.73
Se (196.026 nm)	≤ 2.60	0.95
Zn (213.857 nm)	≤ 1.50	0.31
Pb (220.353 nm)	≤ 2.60	0.73
Mn (257.610 nm)	≤ 1.50	0.39
Al (396.152 nm)	≤ 1.50	0.39
Ba (493.408 nm)	≤ 1.50	0.87
K (766.491 nm)	≤ 1.50	0.32
Axial		
Element Wavelength	Specification	Measured Value % RSD
As (188.980 nm)	≤ 1.50	1.21
Se (196.026 nm)	≤ 1.50	0.84
Zn (206.200 nm)	≤ 1.50	0.56
Zn (213.857 nm)	≤ 1.50	0.96
Cd (214.439 nm)	≤ 1.50	0.26
Pb (220.353 nm)	≤ 1.50	0.51
Mn (257.610 nm)	≤ 1.50	0.97
Cr (267.716 nm)	≤ 1.50	0.22
Cu (324.754 nm)	≤ 1.50	0.24
Al (396.152 nm)	≤ 1.50	0.33
Ba (493.408 nm)	≤ 1.50	0.40
K (766.491 nm)	≤ 1.50	0.65

Page 4 of 4

เอกสารไม่ควบคุม

Report Summary

Instrument Model Agilent 5100/5110 VDV ICP-OES
Instrument ID G8011A/G8015A
Instrument Serial Number MY18030001
Software Version 7.3.1.9507
Firmware Version 3442
Tested By Post Test_PM_Kanyakorn S.
Test Completed On 11/4/2024 11:07:24 AM

Result Summary

Subsystem Communications Test Pass
Air Flow Test Skipped
Water Flow Test Skipped
Gas Flows Test Skipped
RF Generator Test Skipped
Camera Test Skipped
Optics Test Pass
Advanced Valve System Test Skipped
Resolution Test Pass
Sensitivity Test Fail
Precision Test Pass

Subsystem Communications Test Pass

Optics Test

Radial Axial
Intensity 3184054 3177175
Wavelength 737.212 737.212

เอกสารไม่ควบคุม

Resolution Test

Pass

Element Wavelength	Specification	Width
N (174.213 nm)	≤ 9.40	6.97
As (188.980 nm)	≤ 8.20	6.14
C (193.027 nm)	≤ 11.50	8.33
Mo (202.032 nm)	≤ 8.20	6.33
Cr (206.133 nm)	≤ 13.40	9.06
Zn (213.657 nm)	≤ 8.70	6.70
Pb (220.353 nm)	≤ 9.50	7.03
Co (228.615 nm)	≤ 17.20	11.72
Ba (230.424 nm)	≤ 9.40	7.32
Mn (257.610 nm)	≤ 13.30	9.44
Mn (260.568 nm)	≤ 20.30	14.21
Cr (267.716 nm)	≤ 11.00	7.94
Cu (324.754 nm)	≤ 25.00	18.99
Cu (327.395 nm)	≤ 14.20	11.27
Sr (338.071 nm)	≤ 33.50	24.40
Ba (455.403 nm)	≤ 44.00	33.50
Sr (460.793 nm)	≤ 36.00	17.31
Ba (493.408 nm)	≤ 36.00	25.44
Ba (614.171 nm)	≤ 42.00	25.16
Ar (675.283 nm)	≤ 74.00	66.16
K (766.491 nm)	≤ 80.00	65.66

เอกสารไม่ควบคุม

Sensitivity Test

Fail

Radial					
Element Wavelength	Specification	Method	Ratio	Standard	Blank
As (188.980 nm)	≥ 46.0	SRBR	130.6	977.1	50.4
Se (196.026 nm)	≥ 41.0	SRBR	106.0	958.7	70.2
Zn (213.857 nm)	≥ 1421.0	SRBR	4124.8	44037.7	113.4
Pb (220.353 nm)	≥ 46.0	SRBR	207.2	2554.7	136.2
Mn (257.610 nm)	≥ 3518.0	SRBR	13017.8	271840.6	434.7
Al (396.152 nm)	≥ 3.4	SBR	9.7	50615.5	4717.0
Ba (493.408 nm)	≥ 34.0	SBR	133.7	2069203.0	15359.3
K (766.491 nm)	≥ 1.8	SBR	4.8	100199.5	17235.5

Axial					
Element Wavelength	Specification	Method	Ratio	Standard	Blank
As (188.980 nm)	≥ 208.0	SRBR	174.9	1566.7	73.0
Se (196.026 nm)	≥ 159.0	SRBR	167.0	1863.4	110.2
Zn (206.200 nm)	≥ 234.0	SRBR	740.9	6836.0	83.1
Zn (213.857 nm)	≥ 1743.0	SRBR	6965.9	101568.1	211.7
Cd (214.439 nm)	≥ 4227.0	SRBR	5781.0	72852.9	158.1
Pb (220.353 nm)	≥ 320.0	SRBR	501.0	8464.3	267.7
Mn (257.610 nm)	≥ 10625.0	SRBR	31121.6	1006637.8	1044.0
Cr (267.716 nm)	≥ 1048.0	SRBR	4424.8	132202.9	880.8
Cu (324.754 nm)	≥ 19.0	SBR	68.7	302907.8	4345.6
Al (396.152 nm)	≥ 6.0	SBR	21.1	218771.0	9892.3
Ba (493.408 nm)	≥ 60.0	SBR	250.6	7137380.9	28367.3
K (766.491 nm)	≥ 24.0	SBR	45.3	1435050.6	31025.0

เอกสารไม่ควบคุม

Precision Test

Pass

Radial		
Element Wavelength	Specification	Measured Value % RSD
As (188.980 nm)	≤ 2.60	0.81
Se (196.026 nm)	≤ 2.60	0.98
Zn (213.857 nm)	≤ 1.50	0.22
Pb (220.353 nm)	≤ 2.60	0.37
Mn (257.610 nm)	≤ 1.50	0.27
Al (396.152 nm)	≤ 1.50	0.25
Ba (493.408 nm)	≤ 1.50	0.53
K (766.491 nm)	≤ 1.50	0.15

Axial		
Element Wavelength	Specification	Measured Value % RSD
As (188.980 nm)	≤ 1.50	0.81
Se (196.026 nm)	≤ 1.50	0.65
Zn (206.200 nm)	≤ 1.50	0.79
Zn (213.857 nm)	≤ 1.50	0.81
Cd (214.439 nm)	≤ 1.50	0.35
Pb (220.353 nm)	≤ 1.50	0.33
Mn (257.610 nm)	≤ 1.50	1.02
Cr (267.716 nm)	≤ 1.50	0.32
Cu (324.754 nm)	≤ 1.50	0.51
Al (396.152 nm)	≤ 1.50	0.37
Ba (493.408 nm)	≤ 1.50	0.68
K (766.491 nm)	≤ 1.50	0.74

เอกสารไม่ควบคุม

Report Summary		
Instrument Model	Agilent 5100/5110 VDV ICP-OES	
Instrument ID	G8011A/G8015A	
Instrument Serial Number	MY18030001	
Software Version	7.3.1.9507	
Firmware Version	3442	
Tested By	Post Test_PM_Kanyakorn S.	
Test Completed On	11/4/2024 11:30:15 AM	
Result Summary		
Subsystem Communications Test		Pass
Air Flow Test		Pass
Water Flow Test		Pass
Gas Flows Test		Pass
RF Generator Test		Pass
Camera Test		Pass
Optics Test		Skipped
Advanced Valve System Test		Skipped
Resolution Test		Skipped
Sensitivity Test		Skipped
Precision Test		Skipped
Subsystem Communications Test		Pass
Air Flow Test		Pass
30% Air Flow (relative speed)	75% Air Flow (relative speed)	
15.00	19.00	
Water Flow Test		Pass
RF Water Flow(L/min)	Camera Water Flow (L/min)	Water Inlet Temperature (°C)
1.30	0.81	20.55

Page 1 of 2

เอกสารไม่ควบคุม

Gas Flows Test			Pass		
Nebulizer Target Flow	Actual Flow	Back Pressure	Auxiliary Target Flow	Actual Flow	Back Pressure
0.70	0.70	154.65	2.00	2.00	110.92
Makeup Target Flow	Actual Flow	Back Pressure	Plasma Target Flow	Actual Flow	Back Pressure
2.00	2.00	115.38	18.00	17.97	21.48
RF Generator Test			Pass		
RF Power Supply Test	Passed				
RF Power Supply (V)	128.554				
RF Oscillator Test	Passed				
RF Oscillator Frequency (MHz)	25.834				
Work Coil Current (A)	44.660				
RF Power Supply Current (A)	1.999				
Camera Test			Pass		
	Integration Time (ms)	Standard Deviation	Status		
Electronic Offset Test	1000	5.228	Passed		
Dark Current Test	6000	1.168	Passed		
Array Test	5	0.024	Passed		
Linearity Test		0.118	Passed		

Page 2 of 2

เอกสารไม่ควบคุม

Report Summary		
Instrument Model	Agilent 5100/5110 VDV ICP-OES	
Instrument ID	G8011A/G8015A	
Instrument Serial Number	MY18030001	
Software Version	7.3.1.9507	
Firmware Version	3442	
Tested By	change mirror	
Test Completed On	11/8/2024 10:35:26 AM	
Result Summary		
Subsystem Communications Test		Skipped
Air Flow Test		Skipped
Water Flow Test		Skipped
Gas Flows Test		Skipped
RF Generator Test		Skipped
Camera Test		Skipped
Optics Test		Skipped
Advanced Valve System Test		Skipped
Resolution Test		Pass
Sensitivity Test		Pass
Precision Test		Pass

Page 1 of 4

เอกสารไม่ควบคุม

Resolution Test		
Element Wavelength	Specification	Width
N (174.213 nm)	≤ 9.40	6.79
As (188.980 nm)	≤ 8.20	5.80
C (193.027 nm)	≤ 11.50	8.15
Mo (202.032 nm)	≤ 8.20	5.90
Cr (206.158 nm)	≤ 13.40	8.85
Zn (213.857 nm)	≤ 8.70	6.77
Pb (220.353 nm)	≤ 9.50	6.61
Co (228.615 nm)	≤ 17.20	11.79
Ba (230.424 nm)	≤ 9.40	7.25
Mn (257.810 nm)	≤ 13.30	9.47
Mn (260.568 nm)	≤ 20.30	14.50
Cr (267.716 nm)	≤ 11.00	7.91
Cu (324.754 nm)	≤ 25.00	18.72
Cu (327.395 nm)	≤ 14.20	11.09
Sr (338.071 nm)	≤ 33.50	25.39
Ba (455.403 nm)	≤ 44.00	33.09
Sr (460.783 nm)	≤ 36.00	18.54
Ba (493.408 nm)	≤ 36.00	25.74
Ba (614.171 nm)	≤ 42.00	25.23
Ar (675.283 nm)	≤ 74.00	58.92
K (766.491 nm)	≤ 80.00	63.16

Page 2 of 4

เอกสารไม่ควบคุม

Sensitivity Test					
Pass					
Radial					
Element Wavelength	Specification	Method	Ratio	Standard	Blank
As (188.980 nm)	≥ 46.0	SRBR	110.5	868.9	54.3
Se (196.026 nm)	≥ 41.0	SRBR	88.3	934.7	91.3
Zn (213.857 nm)	≥ 1421.0	SRBR	3535.4	44017.7	153.9
Pb (220.353 nm)	≥ 46.0	SRBR	184.5	2492.3	159.8
Mn (257.610 nm)	≥ 3518.0	SRBR	11099.6	249595.3	503.6
Al (396.152 nm)	≥ 3.4	SBR	8.7	50274.4	5172.0
Ba (493.408 nm)	≥ 34.0	SBR	124.5	1903164.1	15166.0
K (766.491 nm)	≥ 1.8	SBR	6.9	110041.4	13991.2
Axial					
Element Wavelength	Specification	Method	Ratio	Standard	Blank
As (188.980 nm)	≥ 208.0	SRBR	253.3	3744.3	196.3
Se (196.026 nm)	≥ 159.0	SRBR	206.7	4199.7	347.2
Zn (206.200 nm)	≥ 234.0	SRBR	923.0	12282.3	172.1
Zn (213.857 nm)	≥ 1743.0	SRBR	6398.3	157551.5	601.7
Cd (214.439 nm)	≥ 4227.0	SRBR	5069.2	99873.7	385.2
Pb (220.353 nm)	≥ 320.0	SRBR	389.0	10641.1	658.6
Mn (257.610 nm)	≥ 10625.0	SRBR	21190.4	985528.7	2153.6
Cr (267.716 nm)	≥ 1048.0	SRBR	3054.1	131797.6	1811.5
Cu (324.754 nm)	≥ 19.0	SBR	36.3	301401.4	8082.9
Al (396.152 nm)	≥ 6.0	SBR	10.8	228359.5	19280.5
Ba (493.408 nm)	≥ 60.0	SBR	106.5	6460421.5	60122.8
K (766.491 nm)	≥ 24.0	SBR	30.2	1639840.6	52562.1

Page 3 of 4

เอกสารไม่ควบคุม

Precision Test			
Pass			
Radial			
Element Wavelength	Specification	Measured Value % RSD	
As (188.980 nm)	≤ 2.60	1.56	
Se (196.026 nm)	≤ 2.60	1.16	
Zn (213.857 nm)	≤ 1.50	0.50	
Pb (220.353 nm)	≤ 2.60	0.74	
Mn (257.610 nm)	≤ 1.50	0.63	
Al (396.152 nm)	≤ 1.50	0.54	
Ba (493.408 nm)	≤ 1.50	0.78	
K (766.491 nm)	≤ 1.50	0.44	
Axial			
Element Wavelength	Specification	Measured Value % RSD	
As (188.980 nm)	≤ 1.50	0.82	
Se (196.026 nm)	≤ 1.50	0.82	
Zn (206.200 nm)	≤ 1.50	0.35	
Zn (213.857 nm)	≤ 1.50	0.34	
Cd (214.439 nm)	≤ 1.50	0.44	
Pb (220.353 nm)	≤ 1.50	0.48	
Mn (257.610 nm)	≤ 1.50	0.83	
Cr (267.716 nm)	≤ 1.50	0.53	
Cu (324.754 nm)	≤ 1.50	0.69	
Al (396.152 nm)	≤ 1.50	0.56	
Ba (493.408 nm)	≤ 1.50	1.29	
K (766.491 nm)	≤ 1.50	0.74	

Page 4 of 4

เอกสารไม่ควบคุม

UNITED ANALYST AND ENGINEERING CONSULTANT COMPANY Ltd.

Automatic Mercury Analyzer

Model RA-4500

Preventive Maintenance Report

Serial No. : 17780278

Soft version : Ver 2.0.7

ROM version : Ver 2.0.1

Date : 09 July 2024

PM by : Pradit Mayong
(Pradit M.)

Approved by : Kitichai S.
(Kitichai S.)



Coax Group Corporation Ltd.

1131/62,64,325-331 Nakornchaisri road,
Kwang ThanonNakornchaisri, Dusit, Bangkok 10300 Thailand
Tel. 02-2435263, 02-6682436 Fax. 02-2437386

เอกสารไม่ควบคุม

Inspection result

ITEM	STANDARD	RESULT	JUDGE
1. Self Check			
1.1 Heating		PASS	OK
1.2 Cooling		PASS	OK
1.3 Leak		PASS	OK
1.4 Optical system		PASS	OK
1.5 Drift		PASS	OK
2. Analytical curve inspection(AREA)			
2.1 No Pretreatment (Low Conc.)	Correlation coefficient (r) ≥ 0.9990	0.9999	OK
3. Repeatability(AREA)			
3.1 No Pretreatment 100ppb, n=3		1. 99.60 ppb 2. 101.84 ppb 3. 101.22 ppb C.V. ≤ 5% 1.15%	OK
4. Blank	Below 1.0 (AREA)	0.1002	OK

เอกสารไม่ควบคุม

Counter


Maintenance

MAIN	SC	Counter	Parameter		
Measurement Count	2567122-09-08	Clear	P1 Subst(H)(2000H)	0909m24-07-08	Clear
Mercury Exhaust Filter Amount(mg)(1500mg)	102-09-08	Clear	P2 Subst(H)(2000H)	0909m24-07-08	Clear
Lamp Active Time(3000h)	1613m24-07-08	Clear	P3 Subst(H)(2000H)	0909m24-07-08	Clear
Membrane Filter Usage Time(2000h)	0558m24-07-08	Clear	P4 Subst(H)(2000H)	0909m24-07-08	Clear
Main Pump Subst(750h)	0959m24-07-08	Clear	P5 Subst(H)(2000H)	0909m24-07-08	Clear
Heating Lamp Time	580923m22-08-08	Clear	P6 Subst(H)(2000H)	0909m24-07-08	Clear
			P7 Subst(H)(2000H)	0909m24-07-08	Clear

Exit


Title : Preventive Maintenance RA-4500 sn:17780278
Date : 2024-07-09
Name : Coax Group
Memo : Calibration Curve 0-10ng

Calib



STD

No.	STD [ppb]	SVOL [mL]	CVOL [mL]	DVOL [mL]	STD [ng]	AREA [ON]	MEAS [ng]	Dev [%]	Note
1	100.000	0.000	5.000	5.000	0.000	0.0846	0.0265	-	
2	100.000	0.025	5.000	5.000	2.500	3.3464	2.5298	1.2	
3	100.000	0.050	5.000	5.000	5.000	6.4170	4.8863	2.3	
4	100.000	0.075	5.000	5.000	7.500	9.8647	7.5322	0.4	
5	100.000	0.100	5.000	5.000	10.000	13.1132	10.0253	0.3	

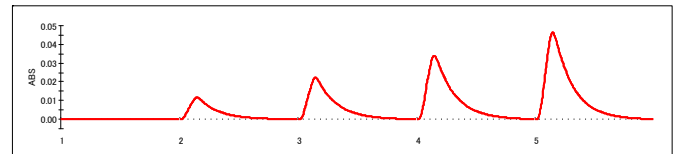

SMP

No.	NAME	SVOL [mL]	CVOL [mL]	DVOL [mL]	AREA [ON]	MEAS [ng]	CONC [ug/L]	Note
1	100ppb	0.050	5.000	5.000	6.5389	4.9798	99.60	
2	100ppb	0.050	5.000	5.000	6.6848	5.0918	101.84	
3	100ppb	0.050	5.000	5.000	6.6446	5.0610	101.22	

Statistics


No.	NAME	TRY	AV [ug/L]	SD [ug/L]	Cv [%]
1	100ppb	3	100.887	1.15660	1.15

เอกสารไม่ควบคุม

-1-

เอกสารไม่ควบคุม

NIPON INSTRUMENTS CORPORATION

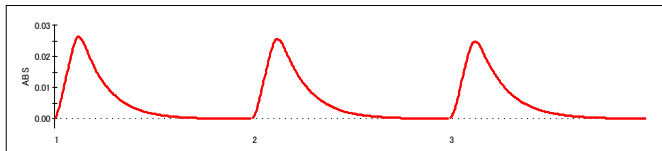


Self Check

Heat check: PASS!! (26.3degC[05:00] -> 30.3degC[02:29])
Sensor check: PASS!! (53- 10- 43)
Leak check: PASS!! (0.19L/min)
Sig./Ref. check: PASS!! (Sig: 4.00V, Ref: 4.02V)
Drift check: PASS!! (0.0000061 - -0.0000179 = 0.0000240)

Title : Preventive Maintenance RA-4500 sn:17780278
Date : 2024-07-09
Name : Coax Group
Memo : Blank

SMP

No.	NAME	SVOL [mL]	CVOL [mL]	DVOL [mL]	AREA [ON]	MEAS [ng]	CONC [ug/L]	Note
1	Blank DI				0.1002	0.0385		

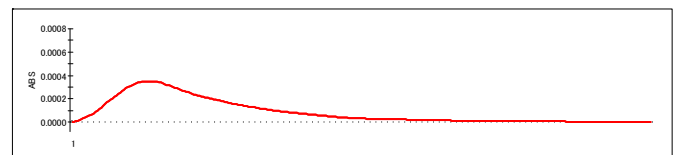

-2-

เอกสารไม่ควบคุม

NIPON INSTRUMENTS CORPORATION

-3-

เอกสารไม่ควบคุม

NIPON INSTRUMENTS CORPORATION

Customer Service Report

FOSS South East Asia 3388 Sirinrat Building, 25th - 26th Floor, Unit No. 3388/90, Rama IV Road, Klongtoey, Klongtoey, Bangkok, Thailand 10110	
Report No.:	13319
Customer:	UAE
Address:	Bangkok
Serial:	91790524
Travel To Customer (Hrs)	Labour (Hrs)
Start 09:00 Finish 10:00	10:00 13:00
Travel From Customer (Hrs)	

Application	Special	Standard
Distributor	Courtesy Visit	Installation
Digital Service	PMA Onboarding	Quote
Internal	Warranty	Repair
Investigate	Sales Support	Remote
		Health Check Visit

PMA Type	Smartcare	Smartcare Pro	Fosscore
	Smartcare Advance	Fosscore Pro	N/A

Details of Work / Test	
- PM -	
+ Visual Check	- ok
- No Leak	- Not ok
- hose damage on heater & main switch	- ok
+ replace heater 10- main switch	- ok
+ replace PM kit #1 set	- ok
+ Function Check	
- heater on/off	- ok
- Alarm	- ok
- Steam	- ok
- Condenser	- ok
Instrument Ready for Use	OK


Part No.	Batch	Description	Qty
100059965	11.06.2022	FOSS PM kit - KT200 heater assembly/2100	1
10005512	29.03.2022	Heater element 8 steam	1
15630111	10.10.2022	Unit for KT200 kit #2 set	1

I confirm this report is accurate and complete	
Signed FOSS	Signed Customer
Name	Name
Email	Customer Contact:
*Remark:	

Agilent CrossLab Start Up Services Agilent 7890 Gas Chromatograph Preventive Maintenance Checklist

Agilent Preventive Maintenance provides factory recommended service for your analytical instruments to assure reliable operation and the accuracy of your results.

Delivered by highly trained and certified service engineers using genuine Agilent parts and supplies, Agilent Preventive Maintenance provides everything you need to reduce unplanned downtime and keep your systems operating at their peak. This checklist will be completed at the end of the service and provided to you as a record of the preventive maintenance activities.



เอกสารไม่ควบคุม



Introduction

Customer Information

- Customers should provide all necessary operating supplies upon request of the engineer.
- A customer representative should be available to the engineer while performing the preventive maintenance procedures.
- Any parts, not included in the Parts Lists section of this document, are not part of the recommended Preventive Maintenance service, nor are they included in the price of this service.
- If a system requires the use of extra or special procedures and/or parts for the maintenance service, then these must be ordered separately and charged as a repair, which may incur additional costs.

Important Customer Web Links

- For more information about **Agilent Technologies services**, please visit our website using the following URL: <http://www.agilent.com/en-us/products/crosslab-instrument-services/service-repair>
- The **Agilent Community** is an excellent place to get answers, collaborate with others about applications and Agilent products, and find in-depth documents and videos relevant to Agilent technologies. Visit <https://community.agilent.com/welcome>.
- To access **Agilent University**, visit <http://www.agilent.com/crosslab/university/> to learn about training options, which include online, classroom and onsite delivery. A training specialist can work directly with you to help determine your best options.
- A useful **Agilent Resource Center** web page is available, which includes short videos on maintenance, quick lists of consumables for new instruments, and other valuable information. Check out the Resource Page here: <https://www.agilent.com/en-us/agilentresources>.
- Need technical support, FAQs, supplies? - visit our **Support Home page** <http://www.agilent.com/search/support>.
- Videos about specific preparation requirements for your instrument can be found by searching the **Agilent YouTube** channel at <https://www.youtube.com/user/agilent>.
- 7890B Manuals** are also available on Agilent.com:
 - Safety** https://www.agilent.com/cs/library/usermanuals/public/7890B_Safety.pdf
 - Installation and First Startup** https://www.agilent.com/cs/library/usermanuals/public/7890B_Installation.pdf
 - Operation Manual** https://www.agilent.com/cs/library/usermanuals/public/7890B_Operation.pdf
 - Maintaining Your GC** https://www.agilent.com/cs/library/usermanuals/public/G3430-90052%207890B_Maintaining%20Guide.pdf



เอกสารไม่ควบคุม



Service Engineer's Responsibilities

- Contact the customer and ensure that all necessary supplies are available before the preventive maintenance visit.
- Only select those pages that relate to the system or module being serviced.
- Complete empty fields with the relevant information.
- Complete the relevant checkboxes in the checklist using either a "X" or tick mark "✓".
- Check "Section not applicable" check boxes to indicate services/tasks not delivered, as appropriate.
- Complete the Preventive Maintenance service in the order of the tasks listed.
- Complete the Service Review section together with the customer.
- Complete the fields for page numbers at the foot of each selected page.
- Complete the total number of pages field in the Service Completion section.
- Ask the customer to sign the Service Completion section including the customer's and your signature.

Additional Instruction Notes

- Check for any active service notes for this unit. If there are any applicable "Safety" or "Modification Recommended" Service notes, plan to implement the changes on this unit before doing any qualification service.
- Do not implement firmware updates, unless you get approval from the customer and are sure that they are compatible with the instrument control software.



เอกสารไม่ควบคุม

System Information

✓ Check this box if an instrument configuration report is attached instead of completing the table below.

Instrument System Name and ID	UAE.TOX.021/2556_CN13113001
Instrument System Site and Location	Room 404

List System Component Product Numbers	List the Serial Numbers of each Component
1. G3440B	CN13113001
2. G4513A	CN22285355
3. G4514A	CN13200169
4.	
5.	
6.	
7.	
8.	
9.	
10.	

Preparation

- ✓ Discuss any specific issues with the customer before starting.
- ✓ Review the instrument logbook for recorded problems and comments.
- ✓ Save instrument control settings before starting the procedure.
- ✓ Perform a general inspection of the system for cleanliness.
- ✓ Check for proper installation of parts, assemblies, sensors etc.
- ✓ Check system for required installation of components, settings as defined by current Service Notes.
- ✓ Check for required firmware updates and verify with customers if they would like them installed.
- ✓ Before starting the following procedures, record the Detector Signal Output(s) in the results table. If the GC is turned OFF or in a service mode, comparing the detector outputs before and after the service is not possible.

Revision: 2.00, Issued: December 30, 2020
 Agile Document Number: D0007063
 DE number: 44166.7597222222
 © Agilent Technologies, Inc. 2020

Page 4 of 9



Preventive Maintenance Procedure

Clean and inspect GC

- ✓ Unplug power cord from the power source.
- ✓ Open GC covers and vacuum/remove any dust/debris. Pay particular attention to cooling fans.
- ✓ Inspect internal connectors for proper contact and placement.
- ✓ Reconnect Power to the GC. Power the GC on and verify the power on self test passed.
- ✓ Verify oven motor spins freely and turns on with the oven door closed; off when the door is opened.
- ✓ Verify operation of all other fans - the inlet and EPC cooling fans.
- ✓ Verify oven intake/outlet flap assembly is operating smoothly while heating and cooling the oven

Inlet and detector consumable replacement

- ✓ For the inlets installed, perform inlet maintenance as defined in the 7890 manual - "Maintaining Your GC" - for the inlet(s) installed.
- ✓ Replace the split vent trap cartridge filter on units with these inlets: Split/Splitless Capillary (SSL), Multi-Mode Inlet (MMI), Programmed Temperature Vaporizer (PTV), Volatiles Interface (VI).
- ✓ If the inlet system is used in Split Mode with viscous samples, inspect and clean the split vent tube on the inlet and flush or replace the tubing between the inlet and the split vent trap.
- ✓ If the GC includes a Flame Ionization Detector (FID), replace the jet. If the ignitor shows any buildup of sample or corrosion, replace the ignitor. Examine the FID collector and castle assemblies for contamination - clean as necessary.

Zero Sensors and Leak test

- ✓ Zero all pressure sensors per the procedure in the 7890 "Advanced User Guide".
- ✓ Perform inlet pressure decay test(s) as defined in the 7890 "Troubleshooting Manual". If the PM is done in preparation for an Operational Qualification, then the pressure decay test defined within that protocol can be used for the PM.
- ✓ Record if test passed or failed in the results table.

Revision: 2.00, Issued: December 30, 2020
 Agile Document Number: D0007063
 DE number: 44166.7597222222
 © Agilent Technologies, Inc. 2020

Page 5 of 9



เอกสารไม่ควบคุม

เอกสารไม่ควบคุม

ALS Maintenance

- ✓ Section NOT applicable
- ✓ Check all cabling and configuration settings between GC, tray, and injectors.
- ✓ Vacuum or remove any dust, especially around fans.
- ✓ Check operation of all fans.
- ✓ Check syringe for smooth plunger operation.
- ✓ Check for smooth operation of the needle support - clean if necessary

Restore Instrument

- ✓ Restore the normal operating conditions or customer method using the Browser interface or Data System.
- ✓ Purge the system with carrier flow for 15 minutes.
- ✓ Bake out the system, then restore the normal operating conditions.
- ✓ After equilibration, check and record the post PM detector signal output values. Results should be similar or lower than the detector outputs recorded prior to PM.
- ✓ Perform a chemical checkout. If this is a routine PM, inject the customer's sample using the ALS if applicable. This will act as a final checkout of both the ALS and the GC.

Note: If the PM Service is performed prior to a qualification service, then use the qualification procedure as a guide for final instrument set up and checkout.

Revision: 2.00, Issued: December 30, 2020
 Agile Document Number: D0007063
 DE number: 44166.7597222222
 © Agilent Technologies, Inc. 2020

Page 6 of 9



Signature Page

Service Review

- ✓ Attach available reports/printouts of all tests to this documentation.
- ✓ Record the Preventive Maintenance service activity in the customer's records/logbook.
- ✓ Update/reset instrument maintenance counters as appropriate.
- ✓ Affix the PM sticker to the system or instrument logbook based on the customer's request.
- ✓ Complete the Service Engineer Comments section if there are additional comments.
- ✓ Review with the customer this service, parts replaced, and test results obtained.
- ✓ If the instrument firmware was updated, record the details of the change in the Service Engineer's Comments box or if necessary, in the customer's IQ records.
- ✓ Supply the customer with a copy of the Smart Alerts flyer.
- ✓ Describe Smart Alerts to the customer.
- ✓ Install Smart Alerts if requested.

7890 GC Test Results Table

Detector Signal Outputs	Before PM Service	After PM Service
Front detector output		24.2
Back detector output		NA.
AUX detector output		NA.
Pressure decay test	Expected test result	Actual test result
Front inlet pressure decay test	Pass	Pass
Back inlet pressure decay test	Pass	NA.

Revision: 2.00, Issued: December 30, 2020
 Agile Document Number: D0007063
 DE number: 44166.7597222222
 © Agilent Technologies, Inc. 2020

Page 7 of 9



เอกสารไม่ควบคุม

เอกสารไม่ควบคุม


7890 Parts List Table

The following kits are recommended for capillary and purged packed inlets. If this is a general PM and the customer has a preferred set of consumables, you may use the customer's consumables.

Part description	Part number	Product or model# where used	Quantity consumed
SSL Capillary Inlet PM kit, Splitless	5188-6497	7890A/B	2
SSL Capillary Inlet PM kit, split	5188-6496	7890A/B	
SSL Capillary Ultra Inert Inlet Gold Seal with Washer	5190-6144	7890A/B	
SSL Capillary Ultra Inert Inlet Splitless Liner - Single taper with Glass Wool	5190-2293	7890A/B	
SSL Capillary Ultra Inert Inlet Low Pressure Drop Split Liner - with Glass Wool	5190-2295	7890A/B	
PP Inlet PM kit	5188-6498	7890A/B	
Split vent trap PM kit, single cartridge (for MMI, PTV & VI)	5188-6495	7890A/B	
MMI Cleaning Kit	G3510-60820	7890A/B	
PTV Septumless Head Rebuild Kit	5182-9747	7890A/B	
PTV Septumless Head Teflon Guide	5182-9748	7890A/B	
Ignitor (glow plug) assembly with O-ring	19231-60680	7890A/B	
FID Collector Rebuild/Cleaning Kit	G1531-67000	7890A/B	
Standard .011-inch FID Jet for capillary FID base	G1531-80560	7890A/B	1
High Temperature .018-inch FID Jet for capillary FID base	G1531-80620	7890A/B	
Standard .018-inch FID Jet for packed column with packed FID base	18710-20119	7890A/B	
Standard .011-inch FID Jet for capillary column with packed/adaptable FID base	19244-80560	7890A/B	
High Temperature .018-inch FID Jet for capillary column with packed/adaptable FID base	19244-80620	7890A/B	
NPD Jet, universal fit, .011-inch ID	G1534-80580	7890A/B	
NPD Jet, universal fit, .011-inch ID Extended tip	G1534-80590	7890A/B	
SSL Capillary Ultra Inert Inlet Gold Seal with Washer	5190-6144	7890A/B	
SSL Capillary Ultra Inert Inlet Splitless Liner - Single taper with Glass Wool	5190-2293	7890A/B	
**FID Collector Replacement Kit, if needed	G1531-67001	7890A/B	

Revision: 2.00, Issued: December 30, 2020
 Agile Document Number: D0007063
 DE number: 44166.759722222
 © Agilent Technologies, Inc. 2020

Page 8 of 9



Service Engineer Comments

If there are any specific points you wish to note as part of performing the service or other items of interest for the customer, please write include them in this box.

Service Completion

Service request number 6006748423 Date service completed 17 April 2024
 Agilent signature Phuwana Customer signature _____
 Total number of pages in this document 9

Revision: 2.00, Issued: December 30, 2020
 Agile Document Number: D0007063
 DE number: 44166.759722222
 © Agilent Technologies, Inc. 2020

Page 9 of 9



เอกสารไม่ควบคุม

เอกสารไม่ควบคุม

Thalunique Co.,Ltd

Open Lab Service for Reliability



THAI UNIQUE OPEN LAB SERVICE

OPERATIONAL QUALIFICATION REPORT (OQ)

Equipment Operational Qualification Report

Report No. SV2407/21898

Equipment GC-MS

System Model SQ

System ID GQS1203F021

Equipment Details Bruker

Test Protocol Scion OQ Protocol

Protocol Rev. A

Date 16-Jul-24

Report Type Report

Org. Name United Analyst and Engineering Consultant Co.,Ltd

Org. Location 3 Soi Udomsuk 41 Sukhumvit Rd.
 Bangkok Phrakhanong Bagkok
 Thailand 10260

เอกสารไม่ควบคุม

เอกสารไม่ควบคุม



CERTIFICATE OF CALIBRATION
GAS CHROMATOGRAPH MASS SPECTROMETER

Certificate No.: SV2407/21898

Customer: United Analyst and Engineering Consultant Co., Ltd.

Address: 3 Soi Udomsuk 41 Sukhumvit Rd. Bangchak
Phrakhanong Bagkok Thailand 10260

Instruments Model: MS Scion-SQ S/N GQS1203F021
GC 451-GC S/N BR1203M099
AUTO SAMPLER CP8400 S/N BR1203M331

Standard Reference Number: 393065201

Procedure Document Number: 394207000

System Test

PM perform and Diagnostic Test	<input checked="" type="checkbox"/> PASS	<input type="checkbox"/> FAIL
Air Water Check Test	<input checked="" type="checkbox"/> PASS	<input type="checkbox"/> FAIL
Tune Test EI	<input checked="" type="checkbox"/> PASS	<input type="checkbox"/> FAIL
Signal to Noise Test (EI) SCAN	<input checked="" type="checkbox"/> PASS	<input type="checkbox"/> FAIL
Injection EI Area Precision Test	<input checked="" type="checkbox"/> PASS	<input type="checkbox"/> FAIL
Injection EI RT Precision Test	<input checked="" type="checkbox"/> PASS	<input type="checkbox"/> FAIL
User Demonstration	<input checked="" type="checkbox"/> PASS	<input type="checkbox"/> FAIL

Engineer 
Somchai Pohongkam

Date 16 July 2024

SCION™

Operational Qualification Protocol

For SCION Instrument

Name and Model:

Serial Number:

System ID Number:

Publication no. 394207000

Revision A

November 2011



Thai Unique Co., Ltd.

Service Division

เอกสารไม่ควบคุม

เอกสารไม่ควบคุม

SCION Operational Qualification Protocol

Contact

Scion Customer Service and Support uses a Customer Relationship Management (CRM) system. The interaction with this system offers the Customer immediate benefits including the contact center or help desk.

Scion worldwide service & support offices can be found from Scion website:



www.scion.com/support.html

Scion is the owner of copyright on this document and any associated software. Under law, the written permission of Scion must be obtained before the documentation or the software is copied, reproduced, translated or converted to electronic or other machine-readable form, in whole, or in part.
First published November 2011.

Scion and the Scion logo are trademarks or registered trademarks of Scion Corporation.

© 2011 Scion

Table of Contents

1.0 Revision History.....	5
2.0 Qualification Representative and Reviewer Details.....	6
2.1 Qualification Representative Details.....	6
2.2 Reviewer Details.....	7
2.3 Quality Assurance/Control Details.....	8
3.0 Customer Responsibilities.....	9
4.0 Qualification Guidelines and GMP Documentation.....	10
4.1 Qualification Summary.....	10
4.2 Qualification Guidelines.....	10
4.3 Page Numbering of Appendices.....	11
4.4 Exception Reports.....	12
4.5 Reference Documents.....	13
4.6 Required Materials.....	14
4.7 General Guidelines.....	15
4.8 Specific Instructions for Documentation.....	15
4.9 Documentation Corrections.....	16
4.10 Marking Procedures Not Applicable.....	16
4.11 Addendums.....	17
4.12 Addendum Example.....	17
5.0 Operational Qualification.....	18
5.1 OQ Preparation.....	18
5.2 System Description.....	20
5.3 Data Sheet Specifications.....	21
5.4 EI Precision Test TQ.....	22
5.5 EI Precision Test SQ.....	23
5.6 Final Evaluation.....	25
6.0 Protocol Approval.....	26
6.1 Protocol Acceptance / Approval by Customer.....	26

6.2 Operational Qualification Protocol Assignment 6.3	27
Protocol Acceptance / Protocol Approval by Scion 6.4	27
Remarks	28
Appendices	29
A.1 Qualification Representative Details	30
B.1 Exceptions	31
Operational Qualification Protocol Certification	36

1.0 Revision History

This qualification protocol is updated as necessary, which includes the event of any regulatory changes to Title 21 of the Code of Federal Regulations (21 CFR) Parts 210 and 211 (if applicable), any software or hardware changes, or updates that may impact on regulatory compliance.

Issue Number	Date	Comments

2.0 Qualification Representative and Reviewer Details


2.1 Qualification Representative Details

Each person responsible for executing any part of this Protocol must complete the table below, providing a sample of their signature and initials, and recording the date the Qualification was performed.

Qualification representatives are nominated to execute and verify the completeness of the test protocol and correctness of all entries.

All testing must be performed in accordance with procedures outlined in this manual. The representative must be trained and qualified to perform the procedures outlined in this document.

A copy of their appropriate qualifications is to be inserted into "Qualification Representative Details" on page 30.

Name (Print)	SOMCHAI POHTONGKAM
Title	ENGINEER
Signature	
Initials	SOMCHAI
Date	16 July 24

Name (Print)	
Title	
Signature	
Initials	
Date	

2.2 Reviewer Details

Each representative responsible for reviewing any part of this protocol must record their details in the following tables, providing a sample of their signature and initials, and recording the date the qualification was performed.

An employee or designee of the company operating the instrument must review these qualification procedures. All calculations and data will be checked by the reviewer. Data review must be performed in accordance with the qualification guidelines "Qualification Guidelines and GMP Documentation" on page 10 and in compliance with current Good Manufacturing Practice (cGMP) as specified by 21 CFR Parts 210 and 211.

Documentation supporting training in the area of data review and cGMP must be carefully maintained and reviewed by the instrument owner.

Reviewer representatives are responsible for reviewing the completeness of the qualification protocol and accuracy of all entries.

Name (Print)	
Title	
Signature	
Initials	
Date	

Name (Print)	
Title	
Signature	
Initials	
Date	

2.3 Quality Assurance/Control Details

As Quality Assurance/Control (QA/QC), who is empowered to approve instrument compliance documents, I approve the procedures in the SCION Operational Qualification Protocol, which I may have amended, I accept the qualification of the Qualification Representative, and I will review and initial the results.

Name (Print)	
Title	
Signature	
Initials	
Date	

Name (Print)	
Title	
Signature	
Initials	
Date	

3.0 Customer Responsibilities

The customer shall ensure that the Preventive Maintenance (PM) or Installation Qualification (IQ) up to point 9.11 is completed. A customer representative should be available at all times during the Operational Qualification Protocol.

Note The Operational Qualification Protocol test procedure should be performed after significant repairs, and at least once a year.

Qualification Rep. Initials	<i>Suh P.</i>	Reviewer Initials		QA/QC Initials	
Date	16 July 24	Date		Date	

4.0 Qualification Guidelines and GMP Documentation

4.1 Qualification Summary

At the end of qualification execution, all tables and data entry fields must be completed and all test results, where specified, must be printed and attached to the protocol.

The Qualification Representative and the Reviewer must sign (signature or initials) and date each page that has a signature field. This represents agreement and acceptance of all data and information on the signed page.

Note Scion does not provide instructions for full Qualification of the personal computer (PC) used to operate the SCION. If further qualification of the PC is required the end-user must contact the PC manufacturer.

Note Scion does not provide full qualification instructions for non-Scion manufactured accessories. Limited instructions may be supplied. If qualification of a non-Scion accessory is required, the end user must contact the accessory manufacturer.

4.2 Qualification Guidelines

The following are general guidelines for performing the qualification tests in accordance with cGMP for the Manufacturing, Processing, Packaging, or Holding of Drugs per 21CFR Parts 210 and 211. Additional local requirements may also apply.

- Read the guidelines before starting the qualification.
- Perform all tests exactly as written.
- Use a pen with permanent blue or black ink unless otherwise specified by company policy.
- Neatly strike out any incorrect words or numbers, made while writing comments or recording results, information or data within this Protocol, with a single line. The word(s) crossed out must remain legible. Write the correction as close as possible to the original entry. Write a brief description of the error. For example, write 'Transcription error' or 'Re-written for clarity'. Initial and date the change.
- Entering initials where a signature is requested, and vice versa is permitted. The exception to this is in 2.0: Qualification Representative and Reviewer Details on page 6, where examples of each person's signature and initials are required.
- Use the date format dd Mon yyyy (e.g. 08 Mar 2011) unless otherwise specified by company policy.

- Complete all tables and data fields to comply with this protocol. Blank fields are not permitted. For items that are not applicable, draw a line through the field, and write 'N/A' (Not Applicable). If entire tables or sections of tables are not applicable, strike a line either through the entire table or the specific area and enter 'N/A'. Complete the signature fields on the page.
- Write 'Pass', 'Fail' or 'N/A' as applicable to the test requirement or outcome.
- Ensure that results and/or specific documents are printed and attached to the specified appendix.
- The Qualification Representative and Reviewer must both sign (signature or initials) and date the signature fields on each page. This represents agreement and acceptance of all data and information on the page.

4.3 Page Numbering of Appendices

Each page that is inserted after the appendix is numbered with the letter of the appendix and a sequential number. The appendix page number must be initialed and dated by both the Qualification Representative and the Reviewer.

For example, pages inserted after Appendix C are numbered

C-1, C-2, C-3... etc. along with the initials and date.

If the reverse of each appendix page is left blank, it should be marked 'N/A' and signed and dated.

When the IQ is complete the total number of pages inserted after each appendix is written on the front page of the respective appendix sheet.

Qualification Rep. Initials	<i>Suh P.</i>	Reviewer Initials		QA/QC Initials	
Date	16 July 24	Date		Date	

4.4 Exception Reports

An exception to the protocol occurs when the observed result differs from the acceptance criteria or expected result.

All exceptions to the protocol must be documented in the Exception Report. The Exception Report includes a detailed description of the exception and resolution by the Qualification Representative.

Each Exception Report shall be issued with a unique identification number in the form ERID-XX-X. This number is generated by the page number on which the exception occurred followed by a sequential number indicating each exception found on the page.

For example, if an exception occurs on page 34, the Exception Report shall be identified as 'ERID-34-1'. If another exception occurs on page 34, the second report shall be identified as 'ERID-34-2'. This identification number should be recorded in the 'Pass / Fail / N/A' field after each test.

Each Exception Report must be signed by the Qualification Representative and the Reviewer as evidence of approval.

The Exception Report is inserted in the appropriately named appendix and numbered as per Section 4.3 of this protocol.

Qualification Rep. Initials	<i>Suh P.</i>	Reviewer Initials		QA/QC Initials	
Date	16 July 24	Date		Date	

4.5 Reference Documents

The following documents are relevant to this Qualification:

- Installation Qualification Protocol
- Completed service report from Preventative Maintenance (PM) schedule

Qualification Rep. Initials	<i>Suh P.</i>	Reviewer Initials		QA/QC Initials	
Date	16 July 24	Date		Date	

4.6 Required Materials

The following stock solutions are required:

- 100 fg/μL OFN 394204200
- 1 pg/μL OFN 393065201
- 100 pg/μL OFN 393110101
- 10 pg/μL BZP 93065301
- 100 pg/μL BZP 394206200

The above solutions will be used to prepare the following working solutions which will be required to execute this OQ:

Note Refer to Appendix 1 for the preparation of the standard solutions.

Qualification Rep. Initials	<i>Suh P.</i>	Reviewer Initials		QA/QC Initials	
Date	16 July 24	Date		Date	

4.7 General Guidelines

The following are general cGMP guidelines.

- Perform each procedure exactly as written.
- Fill in each item on the form or mark it Not Applicable (N/A).
- If an item is marked N/A, initial it and date it.
- The Reviewer reviews and initials all entries recorded by the Qualification Representative.
- Keep all raw data. The Qualification Representative and the Reviewer will initial it, and date it.
- Do not destroy raw data.
- Attach raw data from an instrument, such as the SCION, as an Addendum using the instructions in the following Addendums section.
- If several instruments are qualified simultaneously, reference shared information, such as standard preparation and chemical information, to the document containing the original information by its model and instrument identification number.
- Label all reference standards as required by local regulations.
- Record the time each reference standard was opened.
- Use reference standards within 24 hours of preparation.

Qualification Rep. Initials	<i>Suh P.</i>	Reviewer Initials		QA/QC Initials	
Date	16 July 24	Date		Date	

4.8 Specific Instructions for Documentation

The Reviewer designates specific documentation instructions as follows.

Permanent Ink Color	Blue
Preferred Date Format	16 July 24

If more instructions are required: Use an addendum sheet, write the addendum number, and a brief description.

Qualification Rep. Initials	<i>Suh P.</i>	Reviewer Initials		QA/QC Initials	
Date	16 July 24	Date		Date	

4.9 Documentation Corrections

Note All original entries must remain legible after corrections are made.

1. Draw a line through the incorrect information.
2. Write the correction as close as possible to the original entry, or enter a footnote.
3. Write a brief description of the error. For example, write "transcription error," "rewritten for clarity," or "correcting wrong entry".
4. Initial and date the change.

Qualification Rep. Initials	<i>Sahil P.</i>	Reviewer Initials		QA/QC Initials	
Date	16 July 24	Date		Date	

4.10 Marking Procedures Not Applicable

Some sections may not be relevant for the qualification. To indicate that a procedure or part of a form is unnecessary and that it was not forgotten or inadvertently overlooked:

1. Draw a line through the portion that is not applicable. Write the letters N/A (for not applicable), your initials, and the date near the diagonal line.
2. If a procedural step is unnecessary, select N/A if it is indicated, or write a comment in an Addendum. The Qualification Representative and the Reviewer enter their initials and the date near the line.

Note The Qualification Representative and Reviewer must sign and date all forms, even when part or all of the form is marked N/A.

Qualification Rep. Initials	<i>Sahil P.</i>	Reviewer Initials		QA/QC Initials	
Date	16 July 24	Date		Date	

4.11 Addendums

The following are reasons to complete an addendum sheet:

- A deviation needs documentation.
- Additional information or data needs to be recorded.
- Insufficient space to include the correction on the sheet where the error was made.

Qualification Rep. Initials	<i>Sahil P.</i>	Reviewer Initials		QA/QC Initials	
Date	16 July 24	Date		Date	

4.12 Addendum Example

The following is an example of using an addendum sheet to document a deviation.

If some of the items on the sales order were not present, you could do the following:

1. Use an addendum sheet.
2. Write Instrument Delivery on the Procedure line.
3. Write the addendum page number followed by a letter. For example: page 12A, where 12 is the page and A represents the first addendum on that page.
4. Write the plan to obtain the missing items, which may be the following:
 - Scion notified that Part Number XXXXX and XXXX are missing.
 - Scion replied that the parts are in stock and will be sent overnight. While waiting for the parts to arrive, I will continue to set up the instrument.
5. Review the plan with the Reviewer and make the necessary modifications.
6. Document the arrival of the parts and write that this addendum is resolved. Attach a copy of delivery documents and create addendum pages as required.

Qualification Rep. Initials	<i>Sahil P.</i>	Reviewer Initials		QA/QC Initials	
Date	16 July 24	Date		Date	

5.0 Operational Qualification

This chapter contains the tests to be completed to perform an Operational Qualification for the SCION.

5.1 OQ Preparation

The following must be done before starting the OQ:

1. Preventative Maintenance must have been completed and signed off by the Qualification Representative, Reviewer, and QA/QC person, and attach a copy of the service report and add an addendum number.

Addendum P.M. Protocol

Qualification Rep. Initials	<i>Sahil P.</i>	Reviewer Initials		QA/QC Initials	
Date	16 July 24	Date		Date	

2. OQ must have been completed and signed off by the Qualification Representative, Reviewer, and QA/QC person.

Qualification Rep. Initials	<i>Sahil P.</i>	Reviewer Initials		QA/QC Initials	
Date	16 July 24	Date		Date	

3. The QA/QC person must review, approve, append (if necessary), and sign the Pre-execution Approval.

Qualification Rep. Initials	<i>Sahil P.</i>	Reviewer Initials		QA/QC Initials	
Date	16 July 24	Date		Date	

4. The Qualification Representative and the Reviewer must sign and date the Pre-execution Approval.

Qualification Rep. Initials	<i>Sahil P.</i>	Reviewer Initials		QA/QC Initials	
Date	16 July 24	Date		Date	

5.2 System Description

5.2.1 SCION Description

Installation Date: 2015	Principal Operator:	Phone Number:
Company Information		
Company: United Analyst and Engineering		
Name:	Building:	Installation Site: LAB
Address: 7 Soi Udomsuk 41	Address/Location: Sukhumvit Rd.	
City, State: Bangkok, Prachinang	City, State: Bangkok	
Zip/Country: Thailand	Zip/Country: 10110	
System Description		
SCION: SQ	Serial Number: GQ51203F021	
Sales Order Number:	Sales Order Addendum Number:	
GC		
Module Type: Scion 451	Serial Number: BR1203M099	
AutoSampler		
Module Type: CP8400	Serial Number: BR1203M331	
MS Workstation		
Version: MSWS 8.2.1	Serial Number: 01106-6711-BBQ-450d	
Computer Operating System		
Operating System: Windows 7	Version: Pro	Serial No.: 00346-150-436-158 Pack: -
Computer		
Make: Dell	Model: optiplex	Serial No.: DNNV4HSI
Addendum Number(s): 2. System description		Hard Drive 1TB Size / RAM: 4GB
Qualification Rep. Initials: Sander P.	Reviewer Initials:	QA/QC Initials:
Date: 16 July 24	Date:	Date:

5.3 Data Sheet Specifications

Run these tests after the instrument has pumped down and is leak free. Use the factory methods. Follow the Installation Procedure; complete this section and the appropriate line of the OQ Summary. Print out the methods and results and attach as addendums. Use the factory test column Br-5ms 15m X 250im X 0.25im.

Table 5-1 TQ Specification

Mode	Concentration	Scan Range	Result †	N/A	Pass	Fail	Addendum
EI Full Scan	1 pg OFN	50-300	S/N ≥500:1				
EI MRM	100 fg OFN	272-222	S/N ≥5000:1				
PCI Full Scan‡	10 pg BZP	80-230	S/N ≥50:1				
NCI Full Scan‡	1 pg OFN	200-300	S/N ≥4000:1				

† The Signal-to-Noise ratio S/N values are based on RMS noise figure.

‡ CI tests use methane gas as reagent gas.

For any tests that did not pass, complete an Addendum for each, write the Addendum number and a brief description.

Qualification Rep. Initials: Sander P.	Reviewer Initials:	QA/QC Initials:
Date: 16 July 24	Date:	Date:

Table 5-2 SQ Specification

Mode	Concentration	Scan Range	Result †	N/A	Pass	Fail	Addendum
EI Full Scan	1 pg OFN	50-300	S/N ≥600:1		✓		
PCI Full Scan‡	100 pg BZP	80-230	S/N ≥600:1	✓			
NCI Full Scan‡	200 fg OFN	200-300	S/N ≥1000:1	✓			

Qualification Rep. Initials: Sander P.	Reviewer Initials:	QA/QC Initials:
Date: 16 July 24	Date:	Date:

5.4 EI Precision Test TQ

The following precision tests are for systems with autosamplers only. The test solution is 1 pg/μL OFN test mix part number 393065201.

The following is the required precision for 10 consecutive injections:

Injection	Retention Time	Peak Area
1		
2		
3		
4		
5		
6		
7		
8		
9		
10		
% RSD		

As an alternative, a % RSD summary report from MSWS can be added as an addendum.

Addendum: N/A

	N/A	Pass	Fail	Addendum
Observed Mass is between 271.6 m/z to 272.4 m/z, which is ± 0.4 of the expected m/z.	✓			
Retention Time ≤ 1% Relative Standard Deviation (RSD).	✓			
Peak Area ≤ 10% Relative Standard Deviation (RSD).	✓			

To complete this section use the factory MRM method on the system CD. Print a copy of the method and add as an addendum.

Addendum: N/A

If the hardware is not the same as the factory method, then note this in the addendum and how the hardware available has been configured to compensate. The most common variation here is the sampler, where the Combi Pal has been used instead of the 8400. This will have no impact on results and can be tracked and recorded in the addendum.

5.5 EI Precision Test SQ

The following precision tests are for systems with autosamplers only. The test solution is 1 pg/μL OFN test mix part number 393065201.

The following is the required precision for 10 consecutive injections:

Injection	Retention Time	Peak Area
1	3.645	39800
2	3.643	35585
3	3.640	38804
4	3.642	36679
5	3.641	35202
6	3.642	36225
7	3.641	37711
8	3.642	36452
9	3.642	35329
10	3.643	38639
% RSD	0.038	4.343

As an alternative, a % RSD summary report from MSWS can be added as an addendum.

Addendum:

	N/A	Pass	Fail	Addendum
Observed Mass is between 271.6 m/z to 272.4 m/z, which is ± 0.4 of the expected m/z.		✓		
Retention Time ≤ 1% Relative Standard Deviation (RSD).		✓		
Peak Area ≤ 10% Relative Standard Deviation (RSD).		✓		

To complete this section use the factory Scan method on the system CD. Print a copy of the method and add as an addendum.

Addendum N/A

If the hardware is not the same as the factory method, then note this in the addendum and how the hardware available has been configured to compensate. The most common variation here is the sampler, where the Combi Pal has been used instead of the 8400. This will have no impact on results and can be tracked and recorded in the addendum.

Addendum N/A

5.6 Final Evaluation

	N/A	Pass	Fail	Addendum
Is the equipment in normal operation condition?		✓		
Have all of the OQ requirements been completed?		✓		

Qualification Rep. Initials	<u>Sahel P.</u>	Reviewer Initials		QA/QC Initials	
Date	<u>16 July 24</u>	Date		Date	

6.0 Protocol Approval

6.1 Protocol Acceptance / Approval by Customer

I agree that the procedures and information referenced in this document are applicable.

Instrument(s): Scion 451 SQ with CP8400

Serial Number(s): GQS 1203F021

Sales Order Number:

Company Name: United Analyst and Engineering Consultant Co., Ltd.

I agree that the Operational Qualification Protocol has been satisfactorily completed.	<input checked="" type="checkbox"/>
I confirm that the Operational Qualification Protocol has not been completed, because of these failed (non-passed) items	<input type="checkbox"/>

Authorized Customer Representative

Name (Print)	
Title	
Signature	
Initials	
Date	

6.2 Operational Qualification Protocol Assignment

This Operational Qualification Protocol document is used for:

Operational Qualification Protocol as final test at Scion	<input type="checkbox"/>
Operational Qualification Protocol after Installation Qualification	<input type="checkbox"/>
Operational Qualification Protocol after Preventive Maintenance and OQ completion.	<input checked="" type="checkbox"/>

6.3 Protocol Acceptance / Protocol Approval by Scion

I agree that the procedures and information referenced in this document are applicable.

Instrument(s): Scion 451 SQ with CP8400

Serial Number(s): GQS 1203F21

Sales Order Number:

Company Name: United Analyst and Engineering Consultant Co., Ltd.

Scion Certified Engineer

Name (Print)	SOMCHAI POHTONGKAM
Title	ENGINEER
Signature	<i>Somchai P.</i>
Initials	SOMCHAI
Date	

6.4 Remarks

Agilent Preventive Maintenance Services

**Agilent GCMS
Preventive Maintenance**

Agilent Preventive Maintenance provides factory recommended service for your analytical instruments to assure reliable operation and the accuracy of your results

Delivered by highly trained and certified service engineers using genuine Agilent parts and supplies, Agilent Preventive Maintenance provides what you need to reduce unplanned downtime and keep your systems operating at their peak performance.

This checklist is used as a guide for completing the preventive maintenance tasks. A signed copy of this checklist is provided for your records.

Appendices

Each page that is inserted after the appendix is numbered with the letter of the appendix and a sequential number. The appendix page number must be initialed and dated by both the Qualification Representative and the Reviewer.

For example, pages inserted after Appendix C are numbered C-1, C-2, C-3... etc along with the initials and date.

If the reverse of each appendix page is left blank it should be marked NA and signed and dated.

When the OQ is complete the total number of pages inserted after each appendix is written on the front page of the respective appendix sheet.

Introduction

This checklist covers the following model(s):

Type	Model
SQ	5973 Series MSD
SQ	5975 Series MSD
SQ	5977 Series MSD
TQ	7000 Series MS/MS
TQ	7010 Series MS/MS
QTOF	7200 Series QTOF
QTOF	7250 Series QTOF

Customer Information

- Customers should provide all necessary operating supplies upon request of the engineer.
- A customer representative should be available to the engineer while performing the preventive maintenance procedures. Customers are responsible for regular maintenance and are encouraged to observe the service representative.
- Any parts not included in the Parts Lists section of this document are not part of the recommended Preventive Maintenance service nor are they included in the price of this service.
- If a system requires the use of extra or special procedures and/or parts for the maintenance service, then these must be ordered separately and charged as a repair, which may incur additional costs.

Customer Responsibilities

Customers should ensure that all necessary operating supplies, consumables, and usage-dependent items such as gases, vials, syringes, calibrant solution and solvents required for successful preventive maintenance are available. A customer representative should be available while the preventive maintenance is being performed.

- Complete the relevant checkboxes in the checklist using either a "X" or tick mark "✓".
- Check "Service not applicable" check boxes to indicate services/tasks not delivered, as appropriate.
- Complete the Preventive Maintenance services in order by sections: Review, System Checks, Pump maintenance, Cleaning System and Filters, then System Post Check.
 - The tasks in each section may be completed in the most logical order relevant to the system. Complete the **Service Review** section together with the customer.
- Complete the fields for page numbers at the foot of each selected page.
- Add relevant page numbers to selected pages and complete the total number of pages field in the Service Verification section.
- Complete Signature Page and attach Signature Page to Service Order.

Additional Instruction Notes

- Preventive maintenance is a factory recommended procedure designed to reduce the likelihood of electromechanical failures. Failure to perform preventive maintenance may reduce the long-term reliability of certain instruments and systems. **Two preventative maintenances (PMs) per year are recommended, the Major PM Service will be performed annually with an Interim PM performed 6 months after the Major PM.**

Definition of the Task/Recommended items within the document

Task		Recommended		
Yes	No	Interim	Major	As Needed
✓				
	✓			
		✓		
			✓	
				✓

Yes selected means that the task was done or the part was required.

No selected means that the task was not done or the part was not required.


Interim selected means that this task is recommended to be done at 6-month intervals.

Major selected means that this task is recommended to be done yearly, if the customer would like a service to be done at the 6-month interval then the service could be purchased.

As needed selected means that the task was done, or the part was used as needed. For example, there could be two types of filters that could be used, and this was the one selected.

Revision: A.05, Issued: July 2023
DE Number DE48526731
© Agilent Technologies, Inc. 2023

Page 9 of 10



เอกสารไม่ควบคุม

Important notice for customers

The customer should complete the following before the Support Provider arrives on site:

- Perform an autotune and retain the printed tune report just prior to the start of the PM to verify performance of the equipment.

Note: it is recommended to have the customer run the autotune and tune evaluation prior to the PM and then start the vent cycle so that the instrument will be ready for the service representative.

Important Customer Web Links

- To access Agilent training and education, visit <http://www.agilent.com/chem/training> to learn about training options, which include online, classroom and onsite delivery. A training specialist can work directly with you to help determine your best options.
- To access the **Agilent Resource Center** web page, visit <https://www.agilent.com/en-us/agilentresources>. The following information topics are available:
 - Sample Prep and Containment
 - Chemical Standards
 - Analysis
 - Service and Support
 - Application Workflows

- The **Agilent Community** is an excellent place to get answers, collaborate with others about applications and Agilent products, and find in-depth documents and videos relevant to Agilent technologies. Visit <https://community.agilent.com/welcome>
- Videos about specific preparation requirements for your instrument can be found by searching the **Agilent YouTube** channel at <https://www.youtube.com/user/agilent>
- Need to place a service call?** Flexible Repair Options | Agilent

Service Engineer's Responsibilities

- Contact the customer and ensure that all necessary supplies are available before the preventive maintenance visit.
- Only select those pages that relate to the system or module being serviced.
- Complete empty fields with the relevant information.

Revision: A.05, Issued: July 2023
DE Number DE48526731
© Agilent Technologies, Inc. 2023

Page 4 of 10



เอกสารไม่ควบคุม

Instrument Maintenance

Select the appropriate service to be performed.

- Interim Preventive Maintenance (when available, is typically 6 months or at the request of the customer)
- ✓ Major Preventive Maintenance (Yearly)
- Enhanced Preventive Maintenance (when available, is provided "As needed")

System Information

- ✓ Check this box if an instrument configuration report is attached instead of completing the table.

Instrument System Name and ID	US2009M037
Instrument System Site and Location	United Analyst And Engineering / GCMS

List System Component Product Numbers	List the Serial Numbers of each Component
1. G7077B	US2009M037
2.	
3.	
4.	
5.	
6.	

Preparation

- ✓ Discuss any specific issues with the customer before starting.
- ✓ Review the instrument logbook for recorded problems and comments.
- ✓ Save instrument control settings before starting the procedure.
- ✓ Perform a general inspection of the system for cleanliness.
- ✓ Check for proper installation of parts, assemblies, sensors etc.
- ✓ Check system for required installation of components and implementation of Service Notes
- ✓ Check firmware version(s). Updating to the most current versions is strongly recommended. Verify with the customer before updating.

Revision: A.05, Issued: July 2023
DE Number DE48526731
© Agilent Technologies, Inc. 2023

Page 6 of 10



เอกสารไม่ควบคุม

Preventive Maintenance Procedures

- Service Not Applicable

Interim / Major Preventive Maintenance – GCMS

Yes/No	Interim/Major	Description
✓		Perform general inspection of system for cleanliness.
✓		Discuss any problems the customer is having with the instrument.
✓		Review customer maintenance records and exclude maintenance on recently serviced items.
✓		Review the most recent autotune report. This will give a starting point for evaluating spectral peaks, baseline noise, peak shape, mass assignments and resolution.

Interim / Major Preventive Maintenance – System Checks

- Service Not Applicable

Yes/No	Interim/Major	System Checks
✓		Verify that calibration peaks were seen prior to starting the PM.
✓		Vent the instrument.
✓		Inspect vacuum hoses, pump, exhaust tubing, and power cords for excessive wear.
✓		Visually inspect calibrant levels – PFTBA PFDTD (if appl.), IRM (if appl.). Refill if available.
✓		Look for any obvious external damage or problems.
✓		Clean air intake(s). Cosmetic cover(s) may need to be removed.
✓		Verify system line voltage meets instrument specifications: Yes <input checked="" type="checkbox"/> No <input type="checkbox"/>
✓		For Hydrolert systems, verify customer is running hydrogen: Yes <input type="checkbox"/> No <input type="checkbox"/>

Interim / Major Preventive Maintenance – Wet Mechanical vacuum pumps

- Service Not Applicable

Yes/No	Interim/Major	Wet Mechanical vacuum pumps
✓		Check for evidence of oil leakage. Check pump gasket for leakage.
✓		GC/MS SQ with diffusion pump, drain and replace diffusion pump oil.
✓		Drain and replace mechanical pump oil.
✓		Replace Oil Mist Filter if applicable.

Revision: A.05, Issued: July 2023
DE Number DE48526731
© Agilent Technologies, Inc. 2023

Page 6 of 10



เอกสารไม่ควบคุม

Yes/No					Wet Mechanical vacuum pumps
<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	Discuss with customer the need for more frequent oil changes if the oil is dirty
<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	Don't use mist filters with Chemical Ionization.
<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	Perform anti-suckback valve test. Power on until side plate is held closed, power off and check that side plate holds closed. Visually confirm that no oil returns up vacuum hose.

Interim / Major Preventive Maintenance – Dry Mechanical vacuum pumps - Diaphragm

☒ Service Not Applicable

Yes/No					Dry Mechanical vacuum pumps - Diaphragm
Yes/No	Interim/Major				Description
<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	Check for evidence of poor vacuum – Turbo power demand, poor manifold vacuum, etc.
<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	Clear air flow paths of dust.
<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	If vacuum is poor, then replace the diaphragm pump.
<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	Perform anti-suckback valve test. Power on until side plate is held closed, power off and check that side plate holds closed.

Interim / Major Preventive Maintenance – Dry Mechanical vacuum pumps - Scroll

☒ Service Not Applicable

Yes/No					Dry Mechanical vacuum pumps - Scroll
Yes/No	Interim/Major				Description
<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	Replace the tips seal on the IDP pump.
<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	Check for evidence of poor vacuum – Rough vac pressure, turbo power demand, poor manifold vacuum, etc.
<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	Replace the Exhaust Filter if required.
<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	Discuss with customer the need for more frequent changes, if needed.
<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	Inform customer that pump gas ballast should be installed all the time.
<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	Perform anti-suckback valve test. Power on until side plate is held closed, power off and check that side plate holds closed.

เอกสารไม่ควบคุม

Interim / Major Preventive Maintenance – Cleaning System and Filters

☐ Service Not Applicable

Yes/No	Interim/Major				Cleaning System and Filters
Yes/No	Interim/Major				Description
<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	Fans
<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	Remove dust from fans and vent covers.
<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	Verify fans are functional and that there is enough space around the instrument for proper cooling.
<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	Source cleaning (all sources except HydroInert)
<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	Open analyzer and remove the source.
<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	Disassemble, Clean, Re-assemble source. (7200, also, remove and clean entrance lens)
<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	Re-install source and close analyzer.
<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	HydroInert Source
<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	Source NOT to be abrasively cleaned. No cleaning required at PM. If a decrease in performance is observed, recommend to the customer that filaments, insulators (repeller and extractor), extractor lens, and repeller lens may need to be replaced to restore performance. HydroInert source should not be run with helium carrier.
<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	Filters
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	Replace RMSH-2 Helium gas filter (collision cell gas) – if applicable
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	Replace RMSN-2 Nitrogen gas filter (collision cell gas) – if applicable
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	Replace RMSHY-2 Hydrogen gas filter (HydroInert and JetClean) – if applicable
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	CP17973 – Gas Clean GS/MS Filter (for He, N2 or H2 carrier) – if required
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	5190-9071 – Methane Gas Filter (CI systems) – if applicable

Guidance: Gas filters need to be changed only if required (ie indicating traps show color change, or if Big Universal Trap are approaching saturation based on time installed or number of gas cylinders changed for that trap)

เอกสารไม่ควบคุม

Interim / Major Preventive Maintenance – System Post Check

☐ Service Not Applicable

Yes/No	Interim/Major				System post-check
Yes/No	Interim/Major				Description
<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	Pump system back down. Wait until system stability has been achieved.
<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	Verify system vacuum reading(s) via the gauge controller.
<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	Leak Check
<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	Verify system in manual tune
<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	Compare against previous tune file report(s)
<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	Change to Tune and verify that all temperatures, pressures, and gas flows reach method set points
<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	Check manually that you have calibration peaks.
<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	EI Autotune Performed

Guidance: If the PM Service is performed prior to a qualification service, then use the qualification procedure as a guide for final instrument setup and checkout.

Service Review

- ☒ Attach available reports/printouts of all tests to this documentation.
- ☒ Record the Preventive Maintenance service activity in the customer's records/logbook.
- ☐ Record the PM event in the Smart Alerts logbook, if applicable.
- ☒ Update/reset instrument maintenance counters as appropriate.
- ☒ Affix the PM sticker to the system or instrument logbook based on the customer's request.
- ☒ Complete the Service Engineer Comments section if there are additional comments.
- ☒ Review this service, parts replaced, and test results obtained with the customer.
- ☐ If the instrument firmware was updated, record the details of the change in the Service Engineer's Comments box. Systems in a compliant environment may need additional documentation.
- ☒ Complete Signature Page and attach Signature Page to Service Order.

Test Results

Test Description	Expected Test Result	Actual Test Result
------------------	----------------------	--------------------

เอกสารไม่ควบคุม

Signature Page

Service Engineer Comments (optional)

If there are any specific points you wish to note as part of performing the service review or other items of interest for the customer, please write in this box.

Service Verification

Service Request Number:

Date of Service Completion:

Service Engineer Name:

Customer Name:

Service Engineer Signature:

Total number of pages in this document:

เอกสารไม่ควบคุม

Agilent CrossLab Start Up Services Agilent 8890 Gas Chromatograph Preventive Maintenance Checklist

Agilent Preventive Maintenance provides factory recommended service for your analytical instruments to assure reliable operation and the accuracy of your results.

Delivered by highly trained and certified service engineers using genuine Agilent parts and supplies, Agilent Preventive Maintenance provides everything you need to reduce unplanned downtime and keep your systems operating at their peak. This checklist will be completed at the end of the service and provided to you as a record of the preventive maintenance activities.

Introduction

Customer Information

- Customers should provide all necessary operating supplies upon request of the engineer.
- A customer representative should be available to the engineer while performing the preventive maintenance procedures.
- Any parts, not included in the Parts Lists section of this document, are not part of the recommended Preventive Maintenance service, nor are they included in the price of this service.
- If a system requires the use of extra or special procedures and/or parts for the maintenance service, then these must be ordered separately and charged as a repair, which may incur additional costs.

Important Customer Web Links

- For more information about **Agilent Technologies services**, please visit our website using the following URL: <http://www.agilent.com/en-us/products/crosslab-instrument-services/service-repair>
- The **Agilent Community** is an excellent place to get answers, collaborate with others about applications and Agilent products, and find in-depth documents and videos relevant to Agilent technologies. Visit <https://community.agilent.com/welcome>.
- To access **Agilent University**, visit <http://www.agilent.com/crosslab/university/> to learn about training options, which include online, classroom and onsite delivery. A training specialist can work directly with you to help determine your best options.
- A useful **Agilent Resource Center** web page is available, which includes short videos on maintenance, quick lists of consumables for new instruments, and other valuable information. Check out the Resource Page here: <https://www.agilent.com/en-us/agilentresources>.
- Need technical support, FAQs, supplies? – visit our **Support Home page** <http://www.agilent.com/search/support>.
- Videos about specific preparation requirements for your instrument can be found by searching the **Agilent YouTube** channel at <https://www.youtube.com/user/agilent>.

Service Engineer's Responsibilities

- Contact the customer and ensure that all necessary supplies are available before the preventive maintenance visit.
- Only select those pages that relate to the system or module being serviced.
- Complete empty fields with the relevant information.
- Complete the relevant checkboxes in the checklist using either a "X" or tick mark "✓".
- Check "Section not applicable" check boxes to indicate services/tasks not delivered, as appropriate.
- Complete the Preventive Maintenance service in the order of the tasks listed.
- Complete the Service Review section together with the customer.
- Complete the fields for page numbers at the foot of each selected page
- Complete the total number of pages field in the Service Completion section
- Ask the customer to sign the **Service Completion** section including the customer's and your signature.

Additional Instruction Notes

- Check for any active service notes for this unit. If there are any applicable "Safety" or "Modification Recommended" Service notes, plan to implement the changes on this unit before doing any qualification service.
- Do not implement firmware updates, unless you get approval from the customer and are sure that they are compatible with the instrument control software.

System Information

- ☐ Check this box if an instrument configuration report is attached instead of completing the table below.

Instrument System Name and ID	UN1945A066
Instrument System Site and Location	United Analyst And Engineering / GCMS

List System Component Product Numbers	List the Serial Numbers of each Component
1. 63542A	CN1945A016
2.	
3.	
4.	
5.	
6.	
7.	
8.	
9.	
10.	

Preparation

- ☒ Discuss any specific issues with the customer before starting.
- ☒ Review the instrument logbook for recorded problems and comments.
- ☒ Save instrument control settings before starting the procedure.
- ☒ Perform a general inspection of the system for cleanliness.
- ☒ Check for proper installation of parts, assemblies, sensors etc.
- ☒ Check system for required installation of components, settings as defined by current Service Notes.
- ☒ Check for required firmware updates and verify with customers if they would like them installed.
- ☒ Before starting the following procedures, record the Detector Signal Output(s) in the results table. If the GC is turned OFF or in a service mode, comparing the detector outputs before and after the service is not possible.

Preventive Maintenance Procedure

Clean and inspect GC.

- ☒ Unplug power cord from the power source.
- ☒ Open GC covers and vacuum/remove any dust/debris. Pay particular attention to cooling fans.
- ☒ Inspect internal connectors for proper contact and placement.
- ☒ Reconnect Power to the GC. Power the GC on and verify the power on self-test passed.
- ☒ Verify oven motor spins freely and turns on with the oven door closed; off when the door is opened.
- ☒ Verify operation of all other fans - the inlet and EPC cooling fans.
- ☒ Verify oven intake/outlet flap assembly is operating smoothly while heating and cooling the oven

Inlet and detector consumable replacement

- ☒ Replace the split vent trap cartridge filter using the Maintenance procedure from either the Browser User interfaces on units with these inlets: Split/Splitless Capillary (SSL), Multi-Mode Inlet (MMI), Programmed Temperature Vaporizer (PTV), Volatiles Interface (VI).
- ☒ If the inlet system is used in Split Mode with viscous samples, inspect and clean the split vent tube on the inlet and flush or replace the tubing between the inlet and the split vent trap.
- ☐ For the inlets installed, perform inlet maintenance using the Maintenance procedure from the Browser User interfaces. Record the results. (Leak and Restriction Test)
- ☐ If the GC includes a Flame Ionization Detector (FID), replace the jet. If the ignitor shows any buildup of sample or corrosion, replace the ignitor. Examine the FID collector and castle assemblies for contamination - clean as necessary.

Zero Sensors and Leak test

- ☒ Zero all pressure sensors using the Browser interface.
- ☒ Perform inlet pressure decay test(s) from the diagnostics screen on the Browser User interface. Record if test passed or failed in the results table.

Note: If the PM is done in preparation for an Operational Qualification, then the pressure decay test defined within that protocol can be used for the PM.

เอกสารไม่ควบคุม

ALS Maintenance

☒ Section NOT applicable

- ☐ Check all cabling and configuration settings between GC, tray, and injectors.
- ☐ Vacuum or remove any dust, especially around fans.
- ☐ Check operation of all fans.
- ☐ Check syringe for smooth plunger operation.
- ☐ Check for smooth operation of the needle support - clean if necessary

Restore Instrument

- ☒ Restore the normal operating conditions or customer method using the Browser interface or Data System.
- ☒ Purge the system with carrier flow for 15 minutes
- ☒ Bake out the system, then restore the normal operating conditions
- ☒ After equilibration, check and record the post PM detector signal output values. Results should be similar or lower than the detector outputs recorded prior to PM.
- ☐ Perform a chemical checkout. If this is a routine PM, inject the customer's sample using the ALS if applicable. This will act as a final checkout of both the ALS and the GC.

Note: If the PM Service is performed prior to a qualification service, then use the qualification procedure as a guide for final instrument set up and checkout.

เอกสารไม่ควบคุม

Signature Page

Service Review

- ☐ Attach available reports/printouts of all tests to this documentation.
- ☒ Record the Preventive Maintenance service activity in the customer's records/logbook.
- ☒ Update/reset instrument maintenance counters as appropriate.
- ☒ Affix the PM sticker to the system or instrument logbook based on the customer's request.
- ☒ Complete the Service Engineer Comments section if there are additional comments.
- ☒ Review with the customer this service, parts replaced, and test results obtained.
- ☐ If the instrument firmware was updated, record the details of the change in the Service Engineer's Comments box or if necessary, in the customer's IQ records.
- ☐ Supply the customer with a copy of the Smart Alerts flyer.
- ☐ Describe Smart Alerts to the customer.
- ☐ Install Smart Alerts if requested.

PM Test Results Table

Test description	Before PM Service	After PM Service
Front detector output	N/A	N/A
Back detector output	N/A	N/A
AUX 1 detector output	N/A	N/A
AUX 2 detector output	N/A	N/A
Test description	Expected test result	Actual test result
Leak and Restriction Test after front inlet maintenance	Pass	Pass
Leak and Restriction Test after back inlet maintenance	Pass	N/A
Leak and Restriction Test after front inlet Split Vent Trap replacement	Pass	Pass
Leak and Restriction Test after back inlet Split Vent Trap replacement	Pass	N/A
Front inlet pressure decay test	Pass	Pass
Back inlet pressure decay test	Pass	N/A

เอกสารไม่ควบคุม

PM Parts List Table

Note: The following kits are recommended for capillary and purged packed inlets. If this is a general PM and the customer has a preferred set of consumables, you may use the customer's consumables.

Part description	Part number	Product or model# where used	Quantity consumed
SSL Capillary Inlet PM kit, Splitless	5188-6497	8890 GC	—
SSL Capillary Inlet PM kit, Split	5188-6496	8890 GC	1
SSL Capillary Ultra Inert Inlet Gold Seal with Washer	5190-6144	8890 GC	N/A
SSL Capillary Ultra Inert Inlet Splitless Liner - Single taper with Glass Wool	5190-2293	8890 GC	N/A
SSL Capillary Ultra Inert Inlet Low Pressure Drop Split Liner - with Glass Wool	5190-2295	8890 GC	N/A
PP Inlet PM kit	5188-6498	8890 GC	N/A
Split vent trap PM kit, single cartridge (for MMI, PTV & VI)	5188-6495	8890 GC	N/A
MMI Cleaning Kit	G3510-60820	8890 GC	N/A
PTV Septumless Head Rebuild Kit	5182-9747	8890 GC	N/A
PTV Septumless Head Teflon Guide	5182-9748	8890 GC	N/A
Ignitor (glow plug) assembly with O-ring	19231-60680	8890 GC	N/A
FID Collector Rebuild/Cleaning Kit	G1531-67000	8890 GC	N/A
FID Collector Replacement Kit	G1531-67001	8890 GC	N/A
Standard .011-inch FID Jet	5200-0176	8890 GC	N/A
Universal .018-inch FID Jet	5200-0177	8890 GC	N/A
FPD Ignitor Assy	19256-60800	8890 GC	N/A

เอกสารไม่ควบคุม

Do not include this section/page in the published, customer-facing PDF version.

This page is only relevant for Agilent source documents for document control purposes and is NOT intended for customer viewing. Refer to the SPIFPM checklist Authoring Guide for more information.

Document Control Logs

Revision Log

Revision	Date	Author	Reason for update
Revision of document	Date of issuance	Author of document	Author to describe main features/changes made for this specific revision
1.00	02-Jan-2019	Dave McKenica	Initial Release
2.00	30-Dec-2020	Gary Boardman	Updated New Template and terminology change: Familiarization to Introduction, Create New Agile Document Number: D0007039

Approval Log

Revision	Approver	Title of approver
Add revision number	Add approver name here	Add approver's function or title here
1.00	Suneetha Tippireddy	GC and GCMS Product Support Manager
2.00	Josh Roark	GC and GCMS Product Support Manager

Designated Evaluation Log

Revision	Designated Evaluator (DE)	Title of DE	DE Number
Add revision number	Add name	Add function or title	Add DE number here
2.00	Michael Zumwalt	CrossLab Start Up Services Application Consulting Lead	44166.7597222222

Revision: 2.03, Issued: May 1st 2024
Agile Document Number: D0013610
DE number: 44166.7597222222
© Agilent Technologies, Inc. 2024

Page 10 of 10



เอกสารไม่ควบคุม

Service Engineer Comments

If there are any specific points you wish to note as part of performing the service or other items of interest for the customer, please write include them in this box.

Service Completion

Service request number 6006790785 Date service completed 27 May 2024
Agilent signature [Signature] Customer signature _____
Total number of pages in this document 10 PageRevision: 2.03, Issued: May 1st 2024
Agile Document Number: D0013610
DE number: 44166.7597222222
© Agilent Technologies, Inc. 2024

Page 9 of 10



เอกสารไม่ควบคุม

TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL 0-2717-3000-29 FAX 0-2719-9484

Certificate of Calibration

Cert. No.: 24TM647
Page: 1 of 3

Equipment : Incubator
Manufacturer : Binder
Model : KB 400 E6
Serial No. : 20200000015535
ID No. : UAE.MIC.018/2564
Submitted by : United Analyst and Engineering Consultant Co.,Ltd.
3 Soi Udomsuk 41, Sukhumvit Road,
Bangchak, Phraekhanong,
Bangkok 10290
Location : Microbiology Laboratory (302)
Received Order : 01 April 2024
Calibration Date : 01 April 2024
Ambient Temperature : $(26 \pm 10) ^\circ\text{C}$
Relative Humidity : $(50 \pm 30) \%$
Calibrated by : Man Pattanapongpaiboon
Approved by : [Signature]
Approved Signatory
() Ponpan Paipim
(✓) Suwit Imjai
() Kunchit Promprat
Issue Date : 7 April 2024

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

เอกสารไม่ควบคุม

Equipment : Incubator
Condition As-Received : Used Item
Reference : 2404-0003OC-6Cert. No.: 24TM647
Page: 2 of 3

Procedure Used :-

Calibration were conducted using calibration procedure CP-OT02 based on TLAS G-20 according to direct measurement method with Data Acquisition which connected with Resistance Temperature Detector (RTD).
The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

Instrument	Serial No.	Cert. No.	Traceable	Due Date
1) Data Acquisition	MY49023932	23LM122	TPA	26 Jul 2024

2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certification is traceable to the International System of Unit.


Remark : TPA : Technology Promotion Association (Thailand - Japan)

Result of Calibration :- (*) Without Adjustment

Function of UUC* : Temperature Source

Fresh air setting : Close

Environment during calibration		
	Beginning	Finished
Temp. (°C)	24	24
REL.Humid. (%)	54	57
AC Supply (Volt)	221	223



Probe Installation Details :

	Dimension of Chamber :
a = 10 cm	D = 0.48 m
b = 10 cm	W = 0.65 m
c = 10 cm	H = 1.2 m
	Capacity = 0.37 m ³

Position :	Ref. Std. ID No.:
1	20-16RTD-01
2	20-16RTD-02
3	20-16RTD-03
4	23-16RTD-04
5	22-16RTD-05
6	20-16RTD-06
7	20-16RTD-07
8	22-16RTD-08
9 (ref.)	22-16RTD-09

เอกสารไม่ควบคุม



Equipment : Incubator
Condition As-Received : Used Item
Reference : 2404-0003OC-6
Result of Calibration :- (*) Without Adjustment
Function of UUC* : Temperature Source
Fresh air setting : Close

Cert. No.: 24TM647
Page : 3 of 3

Calibration Point (°C)	UUC* Setting (°C)	UUC* Reading (°C)	Temperature stability (± °C)	Temperature uniformity (°C)	Overall Variation (°C)	Coverage Factor k
35.0	35.0	35.0	0.035	0.19	0.22	2

Calibration Point (°C)	Measured Temperature (°C)									Uncertainty (± °C)
	1	2	3	4	5	6	7	8	9 (ref.)	
35.0	35.000	35.022	34.841	34.851	35.027	35.011	35.023	35.028	35.007	0.30

Average* : The average of 30 values in each position.

Temperature stability : One-half of the greatest maximum difference of measured temperature at any one sensor.

Temperature uniformity : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.

Overall Variation : The Difference of the maximum and minimum measured temperatures throughout observation.

UUC* : Unit Under Calibration

Note : The reported uncertainty of measurement was included stability and excluded uniformity .

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k , providing a level of confidence of approximately 95 %.

-o0o-

เอกสารไม่ควบคุม



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3 : EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLIANG, SUANLIANG BANGKOK 10250
TEL 0-2717-3000-29 FAX:0-2719-9484



Certificate of Calibration

Cert. No.: 24TM650
Page : 1 of 3

Equipment : Incubator
Manufacturer : Memmert
Model : IPP 260
Serial No. : V616.0066
ID No. : UAE.MIC.032/2559
Submitted by : United Analyst and Engineering Consultant Co.,Ltd.
3 Soi Udomsuk 41, Sukhumvit Road,
Bangchak, Phrakhanong,
Bangkok 10260
Location : Microbiology Laboratory (302)
Received Order : 01 April 2024
Calibration Date : 02 - 03 April 2024
Ambient Temperature : (26 ± 10) °C
Relative Humidity : (50 ± 30) %
Calibrated by : Man Pattanapongpaiboon

Approved by :
Approved Signatory

() Ponpan Paipim
(✓) Suwit Imjai
() Kunchit Promprat

Issue Date : 7 April 2024

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

เอกสารไม่ควบคุม



Equipment : Incubator
Condition As-Received : Used Item
Reference : 2404-0003OC-2

Cert. No.: 24TM650
Page : 2 of 3

Procedure Used :-

Calibration were conducted using calibration procedure CP-OT02 based on TLAS G-20 according to direct measurement method with Data Acquisition which connected with Resistance Temperature Detector (RTD).

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

Instrument	Serial No.	Cert. No.	Traceable	Due Date
1) Data Acquisition	MY49023932	23LM122	TPA	26 Jul 2024

2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certification is traceable to the International System of Unit.

Remark : TPA : Technology Promotion Association (Thailand - Japan)


Result of Calibration :- (*) Without Adjustment

Function of UUC* : Temperature Source

Fresh air setting : Close

Environment during calibration		
	Beginning	Finished
Temp. (°C)	25	25
REL.Humid. (%)	57	54
AC Supply (Volt)	221	222

Position :	Ref. Std. ID No.:
1	19-16RTD-01
2	19-16RTD-02
3	19-16RTD-03
4	19-16RTD-04
5	19-16RTD-05
6	19-16RTD-06
7	21-16RTD-07
8	19-16RTD-08
9 (ref.)	19-16RTD-09



Probe Installation Details :

Dimension of Chamber :

a = 5.0 cm	D = 0.50 m
b = 5.0 cm	W = 0.64 m
c = 5.0 cm	H = 0.80 m
	Capacity = 0.26 m ³

เอกสารไม่ควบคุม



Equipment : Incubator
Condition As-Received : Used Item
Reference : 2404-0003OC-2
Result of Calibration :- (*) Without Adjustment
Function of UUC* : Temperature Source
Fresh air setting : Close

Cert. No.: 24TM650
Page : 3 of 3

Calibration Point (°C)	UUC* Setting (°C)	UUC* Reading (°C)	Temperature stability (± °C)	Temperature uniformity (°C)	Overall Variation (°C)	Coverage Factor k
25.0	25.0	25.0	0.053	0.78	1.3	2
36.0	36.0	36.0	0.14	0.57	0.93	2

Calibration Point (°C)	Measured Temperature (°C)									Uncertainty (± °C)
	1	2	3	4	5	6	7	8	9 (ref.)	
25.0	25.596	25.310	25.439	25.412	24.347	24.332	24.313	24.414	24.875	0.30
36.0	35.643	35.965	35.616	35.701	36.239	36.260	36.343	36.357	36.063	0.31

Average* : The average of 30 values in each position.

Temperature stability : One-half of the greatest maximum difference of measured temperature at any one sensor.

Temperature uniformity : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.

Overall Variation : The Difference of the maximum and minimum measured temperatures throughout observation.

UUC* : Unit Under Calibration

Note : The reported uncertainty of measurement was included stability and excluded uniformity .

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k , providing a level of confidence of approximately 95 %.

-o0o-

เอกสารไม่ควบคุม



Certificate of Calibration

Cert. No.: 24TM614
Page : 1 of 3

Equipment : Water Bath
Manufacturer : Memmert
Model : WNE 14
Serial No. : L414.1407
ID No. : UAE.MIC.006/2558
Submitted by : United Analyst and Engineering Consultant Co.,Ltd.
3 Soi Udomsuk 41, Sukhumvit Road,
Bangchak, Phrakhanong,
Bangkok 10260
Location : Microbiology Laboratory (302)
Received Order : 01 April 2024
Calibration Date : 01 April 2024
Ambient Temperature : (26 ± 10) °C
Relative Humidity : (50 ± 30) %
Calibrated by : Preecha Hlahib
Approved by :
() Ponpan Paipim
(✓) Suwit Imjai
() Kunchit Promprat

Issue Date : 25 April 2024

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

เอกสารไม่ควบคุม



Equipment : Water Bath
Condition As-Received : Used Item
Reference : 2404-0003OC-7
Procedure Used :-

Cert. No.: 24TM614
Page : 2 of 3

Calibration were conducted using in-house calibration procedure CP-OT04 according to direct measurement method with Data Acquisition which connected with Industrial Platinum Resistance Thermometer (IPRT).

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

Instrument	Serial No.	Cert. No.	Traceable	Due Date
1) Data Acquisition	MY44073381	23LM95	TPA	19 May 2024

2. This certificate is valid only to the item calibrated on date and place of calibration.
3. This certification is traceable to the International System of Unit.

Remark : TPA : Technology Promotion Association (Thailand - Japan)


Result of Calibration :-

(*) Without Adjustment

Function of UUC* : Temperature Source

Heat transfer medium used : Water

	Environmental		AC Voltage Supply
	(°C)	(%R.H.)	(Volt)
Beginning of Calibration	29	63	222
Finished of Calibration	27	66	221



Front

Position :	Ref. Std. S/N.:
1	4803988-006
2	4803988-007
3	4804539-014
4	4804539-015
5(ref.)	4804539-016

เอกสารไม่ควบคุม



Equipment : Water Bath
Condition As-Received : Used Item
Reference : 2404-0003OC-7
Result of Calibration :- (*) Without Adjustment
Function of UUC* : Temperature Source

Cert. No.: 24TM614
Page : 3 of 3

Calibration point (°C)	UUC* Setting (°C)	UUC* Reading (°C)	Average* Standard Reading (°C)					Uncertainty (± °C)
			1	2	3	4	5 (ref.)	
44.5	44.5	44.5	44.528	44.462	44.470	44.482	44.489	0.15

Calibration point (°C)	Uniformity (°C)	Stability (± °C)	Coverage Factor k
44.5	0.077	0.049	2

Average* : The average of 30 values in each position.

Uniformity : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.

Stability : One-half of the greatest maximum difference of measured temperature at any one probe.

UUC* : Unit Under Calibration

Note : The reported uncertainty of measurement was included stability and excluded uniformity.

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k , providing a level of confidence of approximately 95 %.

-o0o-

เอกสารไม่ควบคุม



Certificate of Calibration

Cert. No.: 24TM616
Page : 1 of 3

Equipment : Water Bath
Manufacturer : Memmert
Model : WNE 14
Serial No. : L414.1410
ID No. : UAE.MIC.007/2558
Submitted by : United Analyst and Engineering Consultant Co.,Ltd.
3 Soi Udomsuk 41, Sukhumvit Road,
Bangchak, Phrakhanong,
Bangkok 10260
Location : Microbiology Laboratory (302)
Received Order : 01 April 2024
Calibration Date : 02 April 2024
Ambient Temperature : (26 ± 10) °C
Relative Humidity : (50 ± 30) %
Calibrated by : Preecha Hlahib
Approved by :
() Ponpan Paipim
(✓) Suwit Imjai
() Kunchit Promprat

Issue Date : 25 April 2024

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

Uncontrolled Documents



Equipment : Water Bath
Condition As-Received : Used Item
Reference : 2404-0003OC-8

Cert. No.: 24TM616
Page : 2 of 3

Procedure Used :-

Calibration were conducted using in-house calibration procedure CP-OT04 according to direct measurement method with Data Acquisition which connected with Industrial Platinum Resistance Thermometer (IPRT).

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

Instrument	Serial No.	Cert. No.	Traceable	Due Date
1) Data Acquisition	MY44073381	23LM95	TPA	19 May 2024

2. This certificate is valid only to the item calibrated on date and place of calibration.
3. This certification is traceable to the International System of Unit.


Remark : TPA : Technology Promotion Association (Thailand - Japan)

Result of Calibration :- (*) Without Adjustment

Function of UUC* : Temperature Source

Heat transfer medium used : Water

	Environmental		AC Voltage Supply
	(°C)	(%R.H.)	(Volt)
Beginning of Calibration	28	63	222
Finished of Calibration	27	69	221



Front

Position :	Ref. Std. S/N.:
1	4803988-006
2	4803988-007
3	4804539-014
4	4804539-015
5(ref.)	4804539-016



Equipment : Water Bath
Condition As-Received : Used Item
Reference : 2404-0003OC-8
Result of Calibration :- (*) Without Adjustment
Function of UUC* : Temperature Source

Cert. No.: 24TM616
Page : 3 of 3

Calibration point (°C)	UUC* Setting (°C)	UUC* Reading (°C)	Average* Standard Reading (°C)					Uncertainty (± °C)
			1	2	3	4	5 (ref.)	
41.0	41.1	41.1	40.988	40.997	41.014	40.996	40.993	0.15
44.5	44.5	44.5	44.474	44.456	44.460	44.458	44.455	0.15

Calibration point (°C)	Uniformity (°C)	Stability (± °C)	Coverage Factor k
41.0	0.100	0.041	2
44.5	0.070	0.047	2

Average* : The average of 30 values in each position.

Uniformity : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.

Stability : One-half of the greatest maximum difference of measured temperature at any one probe.

UUC* : Unit Under Calibration

Note : The reported uncertainty of measurement was included stability and excluded uniformity.

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

Uncontrolled Documents

Uncontrolled Documents

Calibration Certificate

Certificate No.: 2403982-001-01
Client name: UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.
Address: 3 Soi Udomsuk 41, Sukhumvit Road,
Bangchack, Prakhonong, Bangkok 10260

Page 1 of 3.

Equipment: Autoclave
Manufacturer: ALP
Model: CL-40L
Serial No.: 807298
ID No.: UAE.MIC.019/2560
Order No.: 2403982
Operation No.: 2403982-001
Date of Receipt: 7 August 2024
Date of Calibration: 7 August 2024

Calibrated by Mr.Manas Somsak Specialist
Approved by *P. Jaenghailit*
(Miss Praeyaporn Jaengkarnkit)
Vice President, Department of Laboratory Services
Responsible for the Technical Management Team

Date of Issue: 14 August 2024

The uncertainties are for a confidence probability of approximately 95 %.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the National Food Institute.

F-CS-009 Revision: 01 Date: 20-04-65

Calibration Report


Certificate No.: 2403982-001-01
Equipment: Autoclave
Model: CL-40L Serial No.: 807298
Resolution: 1 °C ID No.: UAE.MIC.019/2560
Manufacturer: ALP
Date of Calibration: 7 August 2024

Page 3 of 3

Calibration point: 121 °C

Calibration result:

Calibration Condition	Temperature (°C)	Relative Humidity (%)	Line Voltage (Volt)
Min	28.0	55	224
Max	30.0	65	226



Standard at Position
100F1 = Attached to the food temperature probe, within 20 mm.
100F2 = In the upper part of the chamber.
100F3 = In the chamber door, within 100 mm.

Table 1 : Reporting of Temperature

Calibration Point (°C)	Measured Temperature (°C) @ Sensor No. (Sensor No.2 is REF)			Uncertainty ± (°C)
	Std.# 1	Std.# 2 (Ref)	Std.# 3	
121	122.43	122.44	122.44	0.65

Table 2 : Reporting of Characterization Result

UUC* Setting (°C)	UUC* Reading			Stability ± (°C)	Uniformity (°C)	Overall Variation (°C)
	Min (°C)	Max (°C)	Average (°C)			
122	122	122	122	0.11	0.065	0.14

Note

The quoted uncertainty include " Stability " and " Loading effect (20% of Uniformity)"

UUC* = Unit Under Calibration

Stability = One-half of the greatest maximum difference of measured temperatures at any one sensors, for at least half an hour after reaching steady state.

Uniformity = The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time.

Overall Variation = The difference of the maximum and minimum measured temperatures throughout observation time.

The report uncertainty of measurement was based on standard uncertainty multiplied by coverage factor *k*= 2, providing a level of confidence of approximately 95 %.

----- End -----

F-CS-012 Revision: 01 Date: 20-04-65

Calibration Report

Certificate No.: 2403982-001-01
Equipment: Autoclave
Model: CL-40L Serial No.: 807298
Resolution: 1 °C ID No.: UAE.MIC.019/2560
Manufacturer: ALP
Date of Calibration: 7 August 2024 Page 2 of 3

Location: MICROBIOLOGY LABORATORY (301), UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.
Environment Condition: Ambient Temperature (29 ± 1) °C
Relative Humidity (60 ± 5) %
Line Voltage (225 ± 1) Volt

Condition of this results of Calibration:

- This instrument was calibrated by insert 3 standard Data loggers with RTD into its autoclave and calibration according to W-TE-018 based on BS 2646-1:2021, Autoclaves for sterilization in laboratories
Part 1: Design, construction, safety and performance - Specification.
- The temperature scale used was based on ITS - 90.
- All data show below were final values and the initial data may be obtained upon request.
- Reference Standard Instrument :

Instrument	Model	Serial No.	Certificate No.	Due Date	Through
Digital Thermometer with RTD (Data Logger)	OM-CP-HITEMP-140	Q88555	TE 670230-01	25-Feb-25	NATIONAL FOOD INSTITUTE
	OM-CP-HITEMP-140	R5951	TE 670231-01	25-Feb-25	NATIONAL FOOD INSTITUTE
	OM-CP-HITEMP-140	R56916	TE 670232-01	25-Feb-25	NATIONAL FOOD INSTITUTE

- This certificate is traceable to International System of Units (SI Units).
- This certificate was certified only for the instrument we calibrated.
- This result of calibration was found accurate as shown on date and place of calibration only.
- This standard does not apply to sterilizers or disinfectors used for medical, dental, pharmaceutical.
- Condition of Calibrated item : Good
UUC Description : Setting program function sterilization : STERILIZE/NORMAL
Time of sterilization 15 Minute At 121 °C
- Result of Calibration : ☒ Without adjustment
☐ After adjustment

P. Jangharat
14 Aug. 2024

F-CS-012 Revision: 01 Date: 20-04-65

Calibration Certificate

Certificate No.: 2402281-001-01
Client name: UNITED ANALYST AND ENGINEERING CONSULTANT CO., LTD.
Address: 3 Soi Udomsuk 41, Sukhumvit Road, Bangchack, Prakhonong, Bangkok 10260

Page 1 of 3

Equipment: Autoclave
Manufacturer: ALP
Model: CL-40L
Serial No.: 808763
ID No.: UAE.MIC.026/2563
Order No.: 2402281
Operation No.: 2402281-001
Date of Receipt: 2 April 2024
Date of Calibration: 2 April 2024

Calibrated by Mr.Jerawut Prapawuttipong Scientist Approved by (Mr.Pheraphat Tuanjit) Manager, Division of Calibration Laboratory Responsible for the Technical Management Team
Date of Issue: 9 April 2024

The uncertainties are for a confidence probability of approximately 95 %.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the National Food Institute.

F-CS-009 Revision: 01 Date: 20-04-65

Calibration Report

Certificate No.: 2402281-001-01
Equipment: Autoclave
Model: CL-40L Serial No.: 808763
Resolution: 0.1 °C ID No.: UAE.MIC.026/2563
Manufacturer: ALP
Date of Calibration: 2 April 2024 Page 2 of 3

Location: LABORATORY, UNITED ANALYST AND ENGINEERING CONSULTANT CO., LTD.
Environment Condition: Ambient Temperature (25 ± 1) °C
Relative Humidity (55 ± 7) %
Line Voltage (225 ± 5) Volt

Condition of this results of Calibration:

- This instrument was calibrated by insert 3 standard temperature recorder with RTD into its autoclave and calibration according to W-TE-018 based on BS 2646-1:2021 : Autoclaves for sterilization in laboratories Design, construction, safety and performance Specification.
- The temperature scale used was based on ITS - 90 .
- All data show below were final values and the initial data may be obtained upon request.
- Reference Standard Instrument :

Instrument	Model	Serial No.	Certificate No.	Due Date	Through
Digital Thermometer with RTD (Data Logger)	HiTemp140-2	R54918	TE 660383-01	8 April 2024	NATIONAL FOOD INSTITUTE
	HiTemp140-2	S25601	TE 670033-01	9 November 2024	MAGGETECH INC.
	HiTemp140-2	S25602	TE 670034-01	9 November 2024	MAGGETECH INC.

- This certificate is traceable to International System of Units (SI Units).
- This certificate was certified only for the instrument we calibrated.
- This result of calibration was found accurate as shown on date and place of calibration only.
- This standard does not apply to sterilizers or disinfectors used for medical, dental, pharmaceutical.
- Condition of Calibrated item : Good
UUC Description : Setting program function sterilization : STERILIZE/NORMAL
Time of sterilization 15 Minute At 115.0 and 121.0 °C
- Result of Calibration : ☒ Without adjustment
☐ After adjustment

P. Jangharat


F-CS-012 Revision: 01 Date: 20-04-65

Calibration Report

Certificate No.: 2402281-001-01
Equipment: Autoclave
Model: CL-40L Serial No.: 808763
Resolution: 0.1 °C ID No.: UAE.MIC.026/2563
Manufacturer: ALP
Date of Calibration: 2 April 2024 Page 3 of 3

Calibration point: 115.0 and 121.0 °C

Calibration Condition	Temperature (°C)	Relative Humidity (%)	Line Voltage (Volt)
Min	24.4	48.6	220
Max	25.5	62.1	230



Standard at Position
Date 1 = Attached to the food temperature probe, within 20 mm.
Date 2 = In the upper half of the chamber
Date 3 = In the chamber door, within 100 mm.

Table 1 : Reporting of Temperature

Calibration Point (°C)	Measured Temperature (°C) @ Sensor No. (Sensor No.2 is REF)			Uncertainty ± (°C)
	Std. # 1	Std. # 2 (Ref)	Std. # 3	
115.0	115.28	115.35	115.38	0.64
121.0	121.28	121.36	121.37	0.64

Table 2 : Reporting of Characterization Result

UUC* Setting	UUC* Reading			Stability ± (°C)	Uniformity (°C)	Overall Variation (°C)
	Min (°C)	Max (°C)	Average (°C)			
115.0	115.0	115.1	115.0	0.08	0.13	0.48
121.0	121.0	121.1	121.0	0.12	0.17	0.38

Note

The quoted uncertainty include " Stability " and " Loading effect (20% of Uniformity)"
UUC* = Unit Under Calibration

Stability = One-half of the greatest maximum difference of measured temperatures at any one sensors, for at least half an hour after reaching steady state.

Uniformity = The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time.

Overall Variation = The difference of the maximum and minimum measured temperatures throughout observation time.

The report uncertainty of measurement was based on standard uncertainty multiplied by coverage factor k= 2, providing a level of confidence of approximately 95 %.

----- End -----

F-CS-012 Revision: 01 Date: 20-04-65

Calibration Certificate

Certificate No.: 2402419-001-01
Client name: UNITED ANALYST AND ENGINEERING CONSULTANT CO., LTD.
Address: 3 Soi Udomsuk 41, Sukhumvit Road,
Bangchack, Prakhonong, Bangkok 10260

Page 1 of 3

Equipment: Electronic Balance

Manufacturer: OHAUS

Model: PX623

Serial No.: C236754745

ID No.: UAE.MIC.055/2565

Order No.: 2402419

Operation No.: 2402419-001

Date of Receipt: 19 April 2024

Date of Calibration: 19 April 2024

Calibrated by Mr. Pheraphat Tuanjit
Scientist

Approved by *P. Jengphairat*
(Miss Preeyaporn Jaengkarnkit)
Vice President, Department of Laboratory Services
Responsible for the Technical Management Team

The uncertainties are for a confidence probability of approximately 95%

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full, except with the prior written approval of the National Food Institute.

F-CS-009 Revision: 01 Date: 20-04-65

Calibration Report

Certificate No.: 2402419-001-01
Equipment: Electronic Balance
Model: PX623
Serial No.: C236754745
Capacity: 620 g
Manufacturer: OHAUS
Resolution: 0.001 g
ID No.: UAE.MIC.055/2565

Page 2 of 3

Date of Calibration: 19 April 2024

Environment Condition: Ambient Temperature: 26.0 ± 0.3 °C Relative Humidity: 57 ± 8.4 %

Place of Calibration: Room 301, UNITED ANALYST AND ENGINEERING CONSULTANT CO., LTD.

Condition of Equipment: Good Condition

Condition of This Results of Calibration:

1. Calibration Method: NFI Method W-MA-001 In-House Method based on UKAS Lab 14: 2019

2. Reference Standards:

Reference Standard Model Serial No. Calibrated By Certificate No. Due Date

Standard Weight Class E2 1-500g 15882 TCS M23111825 28 November 2024

Instrument Model Serial No. Calibrated By Certificate No. Due Date

Therm-Hygro Meter 608-H1 NFI.BTH 019/23 Quality Reborn QR24-0492 4 March 2025

3. This certification is traceable to SI UNIT

4. This certificate was certified only for the instrument we calibrated.

5. This result of calibration was found accurate as shown on date and place of calibration only.

Calibration Results:


1. Repeatability of Reading:

Nominal Value (g)	Standard Deviation of Reading (g)
300	0.00067
600	0.0010

2. Off-Center Error:

A mass of 200 g was placed and moved to various position on pan.

The balance reading obtained is given in the table.



1	2	3	4	5	6	(Maximum Difference)
(g)	(g)	(g)	(g)	(g)	(g)	(g)
200.000	200.002	200.001	199.999	200.000	200.000	0.002

F-CS-012 Revision: 01 Date: 20-04-65

Calibration Report

Certificate No.: 2402419-001-01
Equipment: Electronic Balance
Model: PX623
Serial No.: C236754745
Capacity: 620 g
Manufacturer: OHAUS
Resolution: 0.001 g
ID No.: UAE.MIC.055/2565

Date of Calibration: 19 April 2024

Page 3 of 3

Calibration Results: (Continued)

Calibration Range: 0-600 g

Calibration Adjustment: Internal Calibration

3. Departure from Nominal Value:

Nominal Value (g)	Standard Value (g)	Average Reading (g)	Correction (g)	Uncertainty (= g)	Coverage Factor k
Unloaded	0.0000	0.000	0.000	0.00093	2.00
1	1.0000	1.000	0.000	0.00093	2.00
5	5.0000	5.000	0.000	0.00093	2.00
10	10.0000	10.000	0.000	0.00093	2.00
20	20.0000	20.000	0.000	0.00093	2.00
50	50.0000	50.001	-0.001	0.00093	2.00
100	100.0000	100.001	-0.001	0.00094	2.00
200	200.0000	200.001	-0.001	0.0011	2.00
300	300.0000	300.003	-0.003	0.0011	2.00
400	400.0000	400.003	-0.003	0.0012	2.00
500	499.9999	500.003	-0.003	0.0013	2.00
600	599.9999	600.003	-0.002	0.0014	2.00

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k , providing a level of confidence of approximately 95 %.

***** End *****

F-CS-012 Revision: 01 Date: 20-04-65