

ภาคผนวกที่ 4

เอกสารสอบเทียบความถูกต้องของเครื่องมือตรวจวัดคุณภาพสิ่งแวดล้อม

- | | |
|------------|--|
| ลำดับที่ 1 | คุณภาพอากาศในบรรยากาศ |
| ลำดับที่ 2 | คุณภาพอากาศจากปล่อง |
| ลำดับที่ 3 | ระดับเสียงในบรรยากาศทั่วไป |
| ลำดับที่ 4 | ระดับเสียงในที่ทำงาน และระดับเสียงบริเวณอุปกรณ์ที่มีระดับเสียงเกิน 85 เดซิเบล (เอ) |
| ลำดับที่ 5 | คุณภาพน้ำจากระบบบำบัดน้ำเสีย |

**ตารางสรุปรายการเอกสารการสอบเทียบความถูกต้องของเครื่องมือเก็บตัวอย่าง
และเครื่องมือตรวจวิเคราะห์คุณภาพสิ่งแวดล้อม**

รายการตรวจวัด	เครื่องมือเก็บตัวอย่าง	เครื่องมือตรวจวิเคราะห์
	ชื่อเครื่องมือ	ชื่อเครื่องมือ
1. คุณภาพอากาศในบรรยากาศ TSP	High Volume Air Sampler Rec No. Blower No. B02, B09, R07, R13, R16	Digital Balance
PM ₁₀	High Volume PM-10 Air Sampler Rec No. Blower No. B-06, B10, B-17, R10, R15	Digital Balance
SO ₂	SO ₂ Analyzer No. B06, B08, B09, R05 Serial No. 1310957747	SO ₂ Analyzer No.B06, B08, B09, R05 Serial No. 1310957747
NO _x	NO _x Analyzer No. B11, R02, R04, R05 Serial No. CM13090047	NO _x Analyzer No.B11, R02, R04, R05 Serial No. CM13090047
2. คุณภาพอากาศจากปล่อง Total Suspended Particulate	Console No. R04, R05 Pitot Tube No. B38, B45	Digital Balance
Oxides of Nitrogen	Vacuum Gauge	Spectrophotometer
Sulfur Dioxide	Personal Pump SKC No. B68, B71 Rotameter No. H-R02, R03	-
Carbon Monoxide	Personal Pump SKC No. B55, B72 Rotameter No. H-R02, R03	CO Analyzer No. R02
3. ระดับเสียงทั่วไป L _{eq} 5 min, L _{eq} 1 hr, L _{eq} 24 hr, L _{max} , L ₉₀ และ L _{dn}	Acoustic Calibrator Sound Level Meter CR-B02, B06	-
4. ระดับเสียงในสถานประกอบการ L _{eq} 24 hr และ TWA	Acoustic Calibrator Sound Level Meter ACO-B18, R52 NMD-B01, B02, B03, B04, B05, B06, B07, B08, B09, B11, B12, B13, B14, B15, B16, B17	-

ลำดับที่ 1

คุณภาพอากาศในบรรยากาศ



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด

S.P.S. CONSULTING SERVICE CO., LTD.

7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900

7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900

Tel : (662) 939-1370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

High Volume Air Sampler Calibration Report

Calibration Method : Multipoint Orifice Flow Transfer Standard

Model : TE 5025A

S/N : 3611

Calibration Data

High Volume Air Sampler Data		Calibration Data		
Recorder No.	Blower No.	Date	Actual Flowrate (ft ³ /min)	R ²
B01	B01	05/02/2025	y = 1.190x-4.759	0.999
B02	B02	05/02/2025	y = 1.167x-1.802	0.999
B03	B03	03/02/2025	y = 1.142x-3.352	0.997
B04	B04	06/02/2025	y = 1.160x-3.139	0.998
B05	B05	06/02/2025	y = 1.155x-5.601	0.996
B06	B06	06/02/2025	y = 1.150x-1.476	0.999
B07	B07	03/02/2025	y = 1.143x-3.035	0.998
B08	B08	03/02/2025	y = 1.161x-4.459	0.999
B09	B09	05/02/2025	y = 1.177x-3.970	0.996
B10	B10	03/02/2025	y = 1.144x-2.471	0.998
B11	B11	03/02/2025	y = 1.195x-5.384	0.996
B12	B12	04/02/2025	y = 1.168x-4.228	0.998
B13	B13	04/02/2025	y = 1.165x-3.801	0.999
B14	B14	04/02/2025	y = 1.148x-3.248	0.996
B15	B15	04/02/2025	y = 1.173x-4.773	0.997
B16	B16	04/02/2025	y = 1.156x-4.042	0.998
B17	B17	06/02/2025	y = 1.140x-2.730	0.999
B18	B18	06/02/2025	y = 1.171x-4.178	0.999
B19	B19	06/02/2025	y = 1.151x-3.979	0.999
B20	B20	04/02/2025	y = 1.129x-1.255	0.999
B21	B21	04/02/2025	y = 1.132x-3.156	0.999
B22	B22	04/02/2025	y = 1.147x-2.649	0.997
B23	B23	03/02/2025	y = 1.158x-3.223	0.999
B24	B24	05/02/2025	y = 1.144x-3.476	0.997
B25	B25	03/02/2025	Y = 1.071x+1.478	0.997
B26	B26	04/02/2025	y = 1.142x-4.263	0.999
B27	B27	04/02/2025	y = 1.175x-5.192	0.996
B28	B28	04/02/2025	y = 1.173x-5.127	0.999
B29	B29	04/02/2025	y = 1.145x-1.952	0.996
B30	B30	06/02/2025	y = 1.162x-3.062	0.999
B31	B31	03/02/2025	y = 1.182x-5.652	0.998
B32	B32	03/02/2025	y = 1.167x-3.993	0.999
B33	B33	05/02/2025	y = 1.168x-4.451	0.998
B34	B34	05/02/2025	y = 1.127x-3.203	0.999

Calibrated by :

Adul Dangklom
(Mr. Adul Dangklom)

Approved by :

Peera Detudom
(Mr. Peera Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด

S.P.S. CONSULTING SERVICE CO., LTD.

7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900

7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900

Tel : (662) 939-4370-72 Fax : (662) 513-4221 E-mail : sale@spscon.com, www.spscon.com

High Volume Air Sampler Calibration Report

Calibration Method : Multipoint Orifice Flow Transfer Standard

Model : TE 5025A

S/N : 3611

Calibration Data

High Volume Air Sampler Data		Calibration Data		
Recorder No.	Blower No.	Date	Actual Flowrate (ft ³ /min)	R ²
B35	B35	05/02/2025	$y = 1.163x - 3.579$	0.997
B36	B36	05/02/2025	$y = 1.130x - 2.116$	0.999
B37	B37	04/02/2025	$y = 1.146x - 2.265$	0.996
B38	B38	04/02/2025	$y = 1.156x - 6.034$	0.998
B39	B39	03/02/2025	$y = 1.151x - 3.366$	0.998
B40	B40	03/02/2025	$y = 1.174x - 4.582$	0.999
B41	B41	06/02/2025	$y = 1.123x - 1.633$	0.997
B42	B42	03/02/2025	$y = 1.149x - 3.382$	0.997
B43	B43	03/02/2025	$y = 1.137x - 2.074$	0.997
B44	B44	03/02/2025	$y = 1.155x - 1.460$	0.999
R01	R01	04/02/2025	$y = 1.121x - 3.007$	0.999
R02	R02	03/02/2025	$y = 1.159x - 5.099$	0.999
R03	R03	05/02/2025	$y = 1.138x - 2.774$	0.998
R04	R04	05/02/2025	$y = 1.118x - 2.575$	0.999
R05	R05	03/02/2025	$y = 1.136x - 1.720$	0.998
R06	R06	05/02/2025	$y = 1.154x - 2.706$	0.997
R07	R07	03/02/2025	$y = 1.037x + 1.361$	0.999
R08	R08	03/02/2025	$y = 1.146x - 3.762$	0.996
R09	R09	05/02/2025	$y = 1.121x - 2.360$	0.997
R10	R10	05/02/2025	$y = 1.180x - 4.626$	0.999
R11	R11	05/02/2025	$y = 1.147x - 3.861$	0.996
R12	R12	03/02/2025	$y = 1.128x - 4.676$	0.998
R13	R13	04/02/2025	$y = 1.135x - 4.055$	0.999
R14	R14	04/02/2025	$y = 1.153x - 3.122$	0.997
R15	R15	03/02/2025	$y = 1.161x - 5.223$	0.998
R16	R16	03/02/2025	$y = 1.187x - 6.674$	0.999
R17	R17	03/02/2025	$y = 1.120x - 1.730$	0.999
R18	R18	03/02/2025	$y = 1.146x - 2.347$	0.998
R19	R19	06/02/2025	$y = 1.161x - 5.195$	0.999
R20	R20	06/02/2025	$y = 1.134x - 3.449$	0.998

Calibrated by :

Adul Dangklom
(Mr. Adul Dangklom)

Approved by :

Peera Detudom
(Mr. Peera Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด

S.P.S. CONSULTING SERVICE CO., LTD.

7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900

7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chafuchak, Bangkok 10900

Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

High Volume PM-10 Air Sampler Calibration Report

Calibration Method : Multipoint Orifice Flow Transfer Standard

Model : TE 5025A

S/N : 3611

Calibration Data

High Volume PM-10 Data		Calibration Data		
Recorder No.	Blower No.	Date	Actual Flowrate (ft ³ /min)	R ²
B01	B01	04/02/2025	$y = 1.135x - 1.122$	0.996
B02	B02	04/02/2025	$y = 1.140x - 0.728$	0.999
B03	B03	04/02/2025	$y = 1.160x - 3.702$	0.998
B04	B04	05/02/2025	$y = 1.154x - 4.671$	0.999
B05	B05	06/02/2025	$y = 1.151x - 2.705$	0.998
B06	B06	03/02/2025	$y = 1.114x - 1.672$	0.997
B07	B07	03/02/2025	$y = 1.085x + 0.543$	0.996
B08	B08	04/02/2025	$y = 1.149x - 2.014$	0.998
B09	B09	03/02/2025	$y = 1.081x + 0.344$	0.997
B10	B10	03/02/2025	$y = 1.094x - 1.679$	0.997
B11	B11	05/02/2025	$y = 1.137x - 0.690$	0.997
B12	B12	03/02/2025	$y = 1.094x - 1.679$	0.997
B13	B13	03/02/2025	$y = 1.172x - 3.186$	0.998
B14	B14	05/02/2025	$y = 1.160x - 5.111$	0.998
B15	B15	03/02/2025	$y = 1.141x - 2.637$	0.998
B16	B16	04/02/2025	$y = 1.106x + 1.699$	0.998
B17	B17	04/02/2025	$y = 1.105x + 1.676$	0.998
B18	B18	04/02/2025	$y = 1.176x - 3.948$	0.997
B19	B19	04/02/2025	$y = 1.065x + 0.997$	0.998
B20	B20	04/02/2025	$y = 1.163x - 5.103$	0.997
B21	B21	05/02/2025	$y = 1.120x + 0.250$	0.999
B22	B22	06/02/2025	$y = 1.152x - 3.458$	0.998
B23	B23	06/02/2025	$y = 1.149x - 3.696$	0.999
B24	B24	03/02/2025	$y = 1.109x - 1.930$	0.999
B25	B25	03/02/2025	$y = 1.166x - 4.876$	0.998
B26	B26	05/02/2025	$y = 1.118x - 2.223$	0.997
B27	B27	03/02/2025	$y = 1.127x - 3.668$	0.999
B28	B28	04/02/2025	$y = 1.112x - 2.294$	0.999
B29	B29	04/02/2025	$y = 1.155x - 4.309$	0.997
B30	B30	04/02/2025	$y = 1.136x - 2.651$	0.998
B31	B31	03/02/2025	$y = 1.086x + 2.828$	0.999
B32	B32	04/02/2025	$y = 1.099x - 0.279$	0.998
B33	B33	04/02/2025	$y = 1.152x - 4.474$	0.997
B34	B34	04/02/2025	$y = 1.149x - 0.892$	0.997

Calibrated by :

Adul Dangklom
(Mr. Adul Dangklom)

Approved by :

Peera Detudom
(Mr. Peera Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด

S.P.S. CONSULTING SERVICE CO., LTD.

7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chulachak, Bangkok 10900

Tel : (662) 939-4370-72. Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

High Volume PM-10 Air Sampler Calibration Report

Calibration Method : Multipoint Orifice Flow Transfer Standard

Model : TE 5025A

S/N : 3611

Calibration Data

High Volume PM-10 Data		Calibration Data		
Recorder No.	Blower No.	Date	Actual Flowrate (ft ³ /min)	R ²
R01	R01	04/02/2025	y = 1.168x-5.536	0.996
R02	R02	04/02/2025	y = 1.116x-2.200	0.998
R03	R03	03/02/2025	y = 1.160x-5.911	0.997
R04	R04	03/02/2025	y = 1.129x-4.829	0.999
R05	R05	03/02/2025	y = 1.119x-3.825	0.998
R06	R06	05/02/2025	y = 1.125x-1.580	0.997
R07	R07	06/02/2025	y = 1.152x-2.503	0.997
R08	R08	03/02/2025	y = 1.114x-1.275	0.996
R09	R09	03/02/2025	y = 1.130x-4.187	0.999
R10	R10	05/02/2025	y = 1.151x-2.832	0.998
R11	R11	05/02/2025	y = 1.134x-2.692	0.997
R12	R12	05/02/2025	y = 1.158x-4.761	0.996
R13	R13	03/02/2025	y = 1.137x-3.435	0.999
R14	R14	03/02/2025	y = 1.126x-2.499	0.996
R15	R15	04/02/2025	y = 1.111x-3.285	0.999
R16	R16	04/02/2025	y = 1.124x-0.808	0.996
R17	R17	04/02/2025	y = 1.141x-3.412	0.999
R18	R18	03/02/2025	y = 1.115x-3.615	0.998
R19	R19	03/02/2025	y = 1.117x-0.234	0.996
R20	R20	06/02/2025	y = 1.146x-4.675	0.997

Calibrated by :

Adul Dangklom
(Mr. Adul Dangklom)

Approved by :

Peera Detudom
(Mr. Peera Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

CALIBRATION REPORT					
SO ₂ FLUORESCENT ANALYZER					
DATE :	20 April 2025	BRAND :	API	MODEL :	100E
NO.	SO ₂ -B06			SERIAL NO.	3430
Calibrator (Dilution System)					
Brand : Teledyne			Model : 700		
Last Cal. Date : 29 October 2024			Serial No. : 421		
Reference Standard Gas					
Standard Gas : Sulphur Dioxide (SO ₂)			Cylinder No. : A00814SK		
Certified Date : 21 June 2021		Expired Date : 21 June 2029		Cylinder Conc. : 49.8 ppm	
CALIBRATING CONDITION					
Pressure	1011	mmbar	Temp.	24.6	°C
			% RH	50	
CALIBRATION SETTING					
Span	Initial Reading (Before Adj.),PPB			Final Reading (After Adj.),PPB	
Set Point	Expected Concentration	Analyzer Response	%Dif	Analyzer Response	Slope
Zero	0	0.11	-	0	-
SO ₂ Span	400.0	400.1	0.025	400.0	1.013
API Model 100E SO ₂ Analyzer Check list					
Test Values	Observed Value	Units	Nominal Range		
RANGE	500	PPB	0-500		
SAMPLE PRESS	28.4	in-Hg	25-35		
SAMPLE FLOW	658	cc/min	650 ± 10%		
PMT	103.2	mV	-20-150 with Zero Air		
UV LAMP	3032.9	mV	1000-4900		
STR. LGT	61.7	PPB	<100		
DRK PMT	63.2	mV	-50 - 200		
DRK LMP	57.9	mV	-50 - 200		
HVPS	675	V	550-900 constant		
DCPS	2519	mV	2500 ± 200		
RCELL TEMP	50.4	°C	50 ± 1		
BOX TEMP	29.0	°C	5-40		
PMT TEMP	7.2	°C	7 ± 2.0		
SO ₂ Span Conc	400	PPB	20-20,000		
SO ₂ Slope	1.013	-	1.0 ± 0.3		
SO ₂ Offset	22.0	mV	<250		
Stability at Zero	0.1	PPB	<0.2		
Stability at Span	0.2	PPB	0.5% of reading (above 50 ppb)		

Calibrated by :

Adul Dangklom
(Mr.Adul Dangklom)

Approved by :

Peera Detudom
(Mr.Peera Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

CALIBRATION REPORT					
SO ₂ FLUORESCENT ANALYZER					
DATE :	20 April 2025	BRAND :	API	MODEL :	100A
NO.	SO ₂ -B08			SERIAL NO.	1003
Calibrator (Dilution System)					
Brand : Teledyne			Model : 700		
Last Cal. Date : 29 October 2024			Serial No. : 421		
Reference Standard Gas					
Standard Gas : Sulphur Dioxide (SO ₂)			Cylinder No. : A00814SK		
Certified Date : 21 June 2021		Expired Date : 21 June 2029		Cylinder Conc. : 49.8 ppm	
CALIBRATING CONDITION					
Pressure	1011	mmbar	Temp.	24.6	°C
			% RH	50	
CALIBRATION SETTING					
Span	Initial Reading (Before Adj.),PPB			Final Reading (After Adj.),PPB	
Set Point	Expected Concentration	Analyzer Response	%Dif	Analyzer Response	Slope
Zero	0	0.10	-	0	-
SO ₂ Span	400.0	399.7	-0.075	400.0	1.004
API Model 100A SO ₂ Analyzer Check list					
Test Values	Observed Value	Units	Nominal Range		
RANGE	500	PPB	0-500		
SAMPLE PRESS	28.7	in-Hg	25-35		
SAMPLE FLOW	653	cc/min	650 ± 10%		
PMT	103.5	mV	-20-150 with Zero Air		
UV LAMP	3047.1	mV	1000-4900		
STR. LGT	61.5	PPB	<100		
DRK PMT	62.9	mV	-50 - 200		
DRK LMP	57.7	mV	-50 - 200		
HVPS	673	V	550-900 constant		
DCPS	2525	mV	2500 ± 200		
RCELL TEMP	50.2	°C	50 ± 1		
BOX TEMP	29.1	°C	5-40		
PMT TEMP	7.3	°C	7 ± 2.0		
SO ₂ Span Conc	400	PPB	20-20,000		
SO ₂ Slope	1.004	-	1.0 ± 0.3		
SO ₂ Offset	22.1	mV	<250		
Stability at Zero	0.1	PPB	<0.2		
Stability at Span	0.2	PPB	0.5% of reading (above 50 ppb)		

Calibrated by :

Adul Dangklom
(Mr.Adul Dangklom)

Approved by :

Peera Detudom
(Mr.Peera Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spicon.com, www.spicon.com

CALIBRATION REPORT					
SO ₂ FLUORESCENT ANALYZER					
DATE :	20 April 2025	BRAND :	Thermo	MODEL :	43C
NO.	SO2-B09	SERIAL NO.	43C-59325-322		
Calibrator (Dilution System)					
Brand : Teledyne			Model : 700		
Last Cal. Date : 29 October 2024			Serial No. : 421		
Reference Standard Gas					
Standard Gas : Sulphur Dioxide (SO ₂)			Cylinder No. : A00814SK		
Certified Date : 21 June 2021		Expired Date : 21 June 2029		Cylinder Conc. : 49.8 ppm	
CALIBRATING CONDITION					
Pressure	1011	mmbar	Temp.	24.6	°C
			% RH	50	
CALIBRATION SETTING					
Span	Initial Reading (Before Adj.),PPB			Final Reading (After Adj.),PPB	
Set Point	Expected Concentration	Analyzer Response	%Dif	Analyzer Response	
Zero	0	0.11	-	0	
SO ₂ Span	400.0	400.3	0.075	400.0	
INSTRUMENT STATUS					
CHAMBER TEMP	44.2 °C		FLOW	1.0 LPM	
PRESSURE	728.6 mm Hg				

Calibrated by :

Adul Dangklom
(Mr.Adul Dangklom)

Approved by :

Peera Detudom
(Mr.Peera Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

CALIBRATION REPORT					
SO ₂ FLUORESCENT ANALYZER					
DATE :	20 April 2025	BRAND :	API	MODEL :	100E
NO.	SO ₂ -R05			SERIAL NO.	3490
Calibrator (Dilution System)					
Brand : Teledyne			Model : 700E		
Last Cal. Date : 28 October 2024			Serial No. : 201-S		
Reference Standard Gas					
Standard Gas : Sulphur Dioxide (SO ₂)			Cylinder No. : A00814SK		
Certified Date : 21 June 2021		Expired Date : 21 June 2029		Cylinder Conc. : 49.8 ppm	
CALIBRATING CONDITION					
Pressure	1011	mmbar	Temp.	24.6	°C
			% RH	50	
CALIBRATION SETTING					
Span	Initial Reading (Before Adj.),PPB			Final Reading (After Adj.),PPB	
Set Point	Expected Concentration	Analyzer Response	%Dif	Analyzer Response	Slope
Zero	0	0.10	-	0	-
SO ₂ Span	400.0	399.8	-0.050	400.0	1.007
API Model 100E SO ₂ Analyzer Check list					
Test Values	Observed Value	Units	Nominal Range		
RANGE	500	PPB	0-500		
SAMPLE PRESS	28.3	in-Hg	25-35		
SAMPLE FLOW	660	cc/min	650 ± 10%		
PMT	103.2	mV	-20-150 with Zero Air		
UV LAMP	3038.6	mV	1000-4900		
STR. LGT	61.5	PPB	<100		
DRK PMT	63.0	mV	-50 - 200		
DRK LMP	57.7	mV	-50 - 200		
HVPS	671	V	550-900 constant		
DCPS	2526	mV	2500 ± 200		
RCELL TEMP	50.0	°C	50 ± 1		
BOX TEMP	29.3	°C	5-40		
PMT TEMP	7.1	°C	7 ± 2.0		
SO ₂ Span Conc	400	PPB	20-20,000		
SO ₂ Slope	1.007	-	1.0 ± 0.3		
SO ₂ Offset	21.6	mV	<250		
Stability at Zero	0.1	PPB	<0.2		
Stability at Span	0.2	PPB	0.5% of reading (above 50 ppb)		

Calibrated by :

Adul Dangklom
(Mr.Adul Dangklom)

Approved by :

Peera Detudom
(Mr.Peera Detudom)

Job Number :	J092400007	Customer Name :	IRPC
Equipment :	Micro Mobile AQMs	Contact Name :	Khun Wirasak Khumsuk
Model :	Micro Mobile AQMs	Telephone Number :	081-803-0475
Serial Number :	Micro Mobile3	E-mail address/Fax. :	wirasak.k@irpc.co.th
Working Date :	12 April 2025	Working Hour :	4 Hours

Service Report

Working Scope:

รถเคลื่อนที่ AQMs micro#3 หยุดตรวจวัดอากาศ ปิดสถานี อยู่ที่ อนามัยหนองจอก จึงได้เข้าทำการตรวจเช็ค


Physical Checking:

- ตรวจเช็ค Data logger พบว่าทำงานได้ปกติ
- ตรวจเช็ค Diagnostic of all analyzers อยู่ในเกณฑ์ปกติ
- ตรวจเช็ค Reading of all analyzers และ Met sensor พบว่าปกติ
- ตรวจเช็ค เครื่องวัดฝุ่น PM-10 พบว่าทำงานได้ปกติ
- ตรวจเช็ค เครื่อง THC analyzer พบว่าทำงานได้ปกติ
- ตรวจเช็ค การทำงานของระบบไฟฟ้า และ UPS พบว่าทำงานได้ปกติ
- ทำความสะอาดภายในสถานี และ บริเวณรอบสถานี

Correction working:

Part Replacement:Addition Recommended:

-- End --

Serviced by :	ชินรส มุขโรจน์	Serviced Date :	12 April 2025
Approved by:		Approved Date :	12 April 2025



บริษัท คิว-ซี โซลูชั่นส์ จำกัด

7/409 ซอยวิภาวดีรังสิต 36 ถนนวิภาวดีรังสิต แขวงจตุจักร เขตจตุจักร กรุงเทพฯ 10900

โทรศัพท์ : (662) 939-5711 (12 Lines) โทรสาร : (662) 939-4207-8

Website <http://www.qshe.co.th> E-mail-address: info@qshe.co.th

General Checking

Equipment : Micro Mobile AQMS

Model : -

Serial Number : -

Manufacturer : -

Item	Description	Set-Point Value	Status & Value	Remark
	<u>On Mobile</u>			
1	Air conditioner operation	OK	OK	
2	Mobile temperature	25-27 °C	25-27 °C	
3	Lighting system	OK	OK	
4	Lamp in sampling box	OK	OK	
5	Sampling probe	Clean	Clean	
6	Blower	OK	OK	
7	Drain liquid in tank	Drain	Drain	
8	Compressor tank set pressure	80 psi	80 psi	
9	Zero air compressor operation	OK	OK	
10	Silica gel for dry air of NO _x analyzer	OK	OK	
11	UPS 6 KVA	OK	OK	
12	Data logger	OK	OK	
13	Ventilation fan	OK	OK	
14	Power cable	OK	OK	
15	Hydrogen Gas	>500 psi	900/40 psi	
16	Standard gas#1 (NO,SO ₂ ,HC,CO)	>500 psi	400/22 psi	

Note :



บริษัท คิว-ซี โซลูชั่นส์ จำกัด

7/409 ซอยวิภาวดีรังสิต 36 ถนนวิภาวดีรังสิต แขวงจตุจักร เขตจตุจักร กรุงเทพฯ 10900

โทรศัพท์ : (662) 939-5711 (12 Lines) โทรสาร : (662) 939-4207-8

Website <http://www.qshe.co.th> E-mail-address: info@qshe.co.th

SO₂ Analyzer

Equipment : Sulfur Dioxide analyzer.

Model : 43i

Serial Number : 1310957747

Manufacturer : Thermo

Diagnostic test value				
Parameter	Observed value		Unit	Nominal range
	Before	After		
Sample reading			ppb	
Range			ppb	50 to 1000 ppb
Averaging Time			Sec	10 to 300 Sec
Calibration Factors				
SO ₂ BKG. ppb			ppb	0 to 60
SO ₂ COEF			-	1.0 ± 0.3
Instrument Controls				
Temp Compensation			On/Off	On
Pressure Compensation			On/Off	On
Flash Lamp			On/Off	On
Communication setting				
Baud Rate			bps	9600 to 115000
Instrument ID			-	0 to 99
Screen Contrast			%	0 to 100
Service Mode			On/Off	Up to used
Diagnostics				
Voltages				
Motherboard voltages:				
3.3 Supply			Vdc	3.3 +/- 1 Vdc
5.0 Supply			Vdc	5.0 +/- 1 Vdc
15.0 Supply			Vdc	15.0 +/- 1 Vdc
24.0 Supply			Vdc	24.0 +/- 1 Vdc
-3.3 Supply			Vdc	- 3.3 +/- 1 Vdc
Interface board voltages:				
PMT Supply				
Flash Supply				
3.3 Supply			Vdc	3.3 +/- 1 Vd
5.0 Supply			Vdc	5.0 +/- 1 Vdc
15.0 Supply			Vdc	15.0 +/- 1 Vdc
-15.0 Supply			Vdc	-15.0 +/- 1 Vdc
24.0 Supply			Vdc	24.0 +/- 1 Vdc
Temperatures				
Internal			°C	15°C to 45°C
Chamber			°C	45°C ± 2°C
Pressure			mmHg	750 ± 100 mmHg
Flow			L/min	0.5 to 1.00 L/min
Lamp intensity			%	40 – 100 %

Note : หน้าจอมีด มองไม่ชัดเจน



บริษัท คิว-ชี โซลูชันส์ จำกัด

7/409 ซอยวิภาวดีรังสิต 36 ถนนวิภาวดีรังสิต แขวงจตุจักร เขตจตุจักร กรุงเทพฯ 10900

โทรศัพท์ : (662) 939-5711 (12 Lines) โทรสาร : (662) 939-4207-8

Website <http://www.qshe.co.th> E-mail-address: info@qshe.co.th



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด

S.P.S. CONSULTING SERVICE CO., LTD.

7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900

7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900

Tel : (662) 939-4370-72 Fax : (662) 513-4221 E-mail : sale@spscon.com, www.spscon.com

CALIBRATION REPORT					
CHEMILUMINESCENT NO / NO ₂ / NO _x ANALYZER					
DATE :	20 April 2025	BRAND :	API	MODEL :	200E
NO.	NOX-B11	SERIAL NO.	4467		
Calibrator (Dilution System)					
Brand	: Teledyne			Model	: 700
Last Cal. Date	: 29 October 2024			Serial No.	: 421
Reference Standard Gas					
Standard Gas	: Nitric Oxide (NO)			Cylinder No.	: A00726SV
Certified Date	: 05 January 2023	Expired Date	: 05 January 2026	Cylinder Conc.	: 48.8 ppm
CALIBRATING CONDITION					
Pressure	1011	mmbar	Temp.	24.6	°C
			% RH	50	
CALIBRATION SETTING					
Span	Initial Reading (Before Adj.),PPB			Final Reading (After Adj.),PPB	
Set Point	Expected Concentration	Analyzer Response	%Dif	Analyzer Response	Slope
Zero	0	0.10	-	0	-
NO Span	400	399.9	-0.025	400.0	1.010
NO _x Span	400	400.2	0.050	400.0	1.013
API Model 200E NO _x Analyzer Check List					
Test Values	Observed Value	Units	Nominal Range		
RANGE	500	PPB	500 standard		
STABILITY (Zero Gas)	0.1	PPB	< 2 with zero air		
SAMPLE FLOW	512	cc/min	500 ± 50		
OZONE FLOW	79	cc/min	80 ± 15		
PMT	102.9	mV	-20 - 150		
AZERO	93.7	mV	-20 - 150		
HVPS	674	V	420 - 900 constant		
RCELL TEMP	50.3	°C	50 ± 1		
BOX TEMP	29.0	°C	8 - 48		
PMT TEMP	7.5	°C	7 ± 2		
MOLY TEMP	315.3	°C	315 ± 5		
RCELL PRESS	8.4	IN-Hg-A	2 - 10 constant		
SAMPLE PRESS	28.7	IN-Hg-A	25 - 30 constant		
NO Span Conc	400	PPB	20 - 20,000		
NO _x Span Conc	400	PPB	20 - 20,000		
NO Slope	1.010	-	1.0 ± 0.3		
NO _x Slope	1.013	-	1.0 ± 0.3		
NO Offset	1.3	mV	-20 to +150		
NO _x Offset	0.9	mV	-20 to 150		
Stability at Zero	0.1	PPB	< 0.2		
Stability at Span	0.2	PPB	< 2 ppb @ 400 ppb span gas		

Calibrated by :

Adul Dangklom
(Mr.Adul Dangklom)

Approved by :

Peera Detudom
(Mr.Peera Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด

S.P.S. CONSULTING SERVICE CO., LTD.

7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900

7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900

Tel : (662) 939-4370-72 Fax : (662) 513-4221 E-mail : sale@spscon.com www.spscon.com

CALIBRATION REPORT

CHEMILUMINESCENT NO / NO₂ / NO_x ANALYZER

DATE : 20 April 2025

BRAND : API

MODEL : 200E

NO. NOX-R02

SERIAL NO. 2285

Calibrator (Dilution System)

Brand : Teledyne

Model : 700E

Last Cal. Date : 28 October 2024

Serial No. : 201-S

Reference Standard Gas

Standard Gas : Nitric Oxide (NO)

Cylinder No. : A00726SV

Certified Date : 05 January 2023

Expired Date : 05 January 2026

Cylinder Conc. : 48.8 ppm

CALIBRATING CONDITION

Pressure 1011 mmbar

Temp. 24.6 °C

% RH 50

CALIBRATION SETTING

Span	Initial Reading (Before Adj.),PPB			Final Reading (After Adj.),PPB	
	Expected Concentration	Analyzer Response	%Dif	Analyzer Response	Slope
Zero	0	-0.10	-	0	-
NO Span	400	399.9	-0.025	400.0	1.007
NO _x Span	400	400.2	0.050	400.0	1.011

API Model 200E NO_x Analyzer Check List

Test Values	Observed Value	Units	Nominal Range
RANGE	500	PPB	500 standard
STABILITY (Zero Gas)	0.1	PPB	< 2 with zero air
SAMPLE FLOW	509	cc/min	500 ± 50
OZONE FLOW	79	cc/min	80 ± 15
PMT	103.2	mV	-20 - 150
AZERO	94.1	mV	-20 - 150
HVPS	669	V	420 - 900 constant
RCELL TEMP	50.3	°C	50 ± 1
BOX TEMP	29.4	°C	8 - 48
PMT TEMP	7.1	°C	7 ± 2
MOLY TEMP	315.3	°C	315 ± 5
RCELL PRESS	8.2	IN-Hg-A	2 - 10 constant
SAMPLE PRESS	28.5	IN-Hg-A	25 - 30 constant
NO Span Conc	400	PPB	20 - 20,000
NO _x Span Conc	400	PPB	20 - 20,000
NO Slope	1.007	-	1.0 ± 0.3
NO _x Slope	1.011	-	1.0 ± 0.3
NO Offset	1.6	mV	-20 to +150
NO _x Offset	1.0	mV	-20 to 150
Stability at Zero	0.1	PPB	< 0.2
Stability at Span	0.2	PPB	< 2 ppb @ 400 ppb span gas

Calibrated by :

Adul Dangklom

(Mr.Adul Dangklom)

Approved by :

Peera Detudom

(Mr.Peera Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด

S.P.S. CONSULTING SERVICE CO., LTD.

7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900

7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900

Tel : (662) 939-4370-72 Fax : (662) 513-4221 E-mail : sale@spscon.com. www.spscon.com

CALIBRATION REPORT					
CHEMILUMINESCENT NO / NO ₂ / NO _x ANALYZER					
DATE :	20 April 2025	BRAND :	API	MODEL :	200E
NO.	NOX-R04	SERIAL NO.	4411		
Calibrator (Dilution System)					
Brand	: Teledyne			Model	: 700E
Last Cal. Date	: 28 October 2024			Serial No.	: 201-S
Reference Standard Gas					
Standard Gas	: Nitric Oxide (NO)			Cylinder No.	: A00726SV
Certified Date	: 05 January 2023	Expired Date	: 05 January 2026	Cylinder Conc.	: 48.8 ppm
CALIBRATING CONDITION					
Pressure	1011	mmbar	Temp.	24.6	°C
% RH	50				
CALIBRATION SETTING					
Span	Initial Reading (Before Adj.),PPB			Final Reading (After Adj.),PPB	
Set Point	Expected Concentration	Analyzer Response	%Dif	Analyzer Response	Slope
Zero	0	-0.10	-	0	-
NO Span	400	399.5	-0.125	400.0	1.003
NO _x Span	400	399.8	-0.050	400.0	1.007
API Model 200E NO _x Analyzer Check List					
Test Values	Observed Value	Units	Nominal Range		
RANGE	500	PPB	500 standard		
STABILITY (Zero Gas)	0.1	PPB	< 2 with zero air		
SAMPLE FLOW	507	cc/min	500 ± 50		
OZONE FLOW	78	cc/min	80 ± 15		
PMT	102.9	mV	-20 - 150		
AZERO	93.7	mV	-20 - 150		
HVPS	674	V	420 - 900 constant		
RCELL TEMP	50.2	°C	50 ± 1		
BOX TEMP	29.3	°C	8 - 48		
PMT TEMP	7.4	°C	7 ± 2		
MOLY TEMP	315.1	°C	315 ± 5		
RCELL PRESS	8.3	IN-Hg-A	2 - 10 constant		
SAMPLE PRESS	28.5	IN-Hg-A	25 - 30 constant		
NO Span Conc	400	PPB	20 - 20,000		
NO _x Span Conc	400	PPB	20 - 20,000		
NO Slope	1.003	-	1.0 ± 0.3		
NO _x Slope	1.007	-	1.0 ± 0.3		
NO Offset	1.0	mV	-20 to +150		
NO _x Offset	0.5	mV	-20 to 150		
Stability at Zero	0.1	PPB	< 0.2		
Stability at Span	0.2	PPB	< 2 ppb @ 400 ppb span gas		

Calibrated by :

Adul Dangklom

(Mr.Adul Dangklom)

Approved by :

Peera Detudom

(Mr.Peera Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด

S.P.S. CONSULTING SERVICE CO., LTD.

7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900

7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900

Tel : (662) 939-4370-72 Fax : (662) 513-4221 E-mail : sale@spscon.com. www.spscon.com

CALIBRATION REPORT					
CHEMILUMINESCENT NO / NO ₂ / NO _x ANALYZER					
DATE :	20 April 2025	BRAND :	API	MODEL :	200E
NO.	NOX-R05	SERIAL NO.	4413		
Calibrator (Dilution System)					
Brand	: Teledyne			Model	: 700E
Last Cal. Date	: 28 October 2024			Serial No.	: 201-S
Reference Standard Gas					
Standard Gas	: Nitric Oxide (NO)			Cylinder No.	: A00726SV
Certified Date	: 05 January 2023	Expired Date	: 05 January 2026	Cylinder Conc.	: 48.8 ppm
CALIBRATING CONDITION					
Pressure	1011	mmbar	Temp.	24.6	°C
% RH	50				
CALIBRATION SETTING					
Span	Initial Reading (Before Adj.),PPB			Final Reading (After Adj.),PPB	
Set Point	Expected Concentration	Analyzer Response	%Dif	Analyzer Response	Slope
Zero	0	0.11	-	0	-
NO Span	400	399.7	-0.075	400.0	1.006
NO _x Span	400	400.2	0.050	400.0	1.009
API Model 200E NO _x Analyzer Check List					
Test Values	Observed Value	Units	Nominal Range		
RANGE	500	PPB	500 standard		
STABILITY (Zero Gas)	0.1	PPB	< 2 with zero air		
SAMPLE FLOW	505	cc/min	500 ± 50		
OZONE FLOW	78	cc/min	80 ± 15		
PMT	103.0	mV	-20 - 150		
AZERO	93.7	mV	-20 - 150		
HVPS	670	V	420 - 900 constant		
RCELL TEMP	50.3	°C	50 ± 1		
BOX TEMP	29.5	°C	8 - 48		
PMT TEMP	7.1	°C	7 ± 2		
MOLY TEMP	314.8	°C	315 ± 5		
RCELL PRESS	8.3	IN-Hg-A	2 - 10 constant		
SAMPLE PRESS	28.6	IN-Hg-A	25 - 30 constant		
NO Span Conc	400	PPB	20 - 20,000		
NO _x Span Conc	400	PPB	20 - 20,000		
NO Slope	1.006	-	1.0 ± 0.3		
NO _x Slope	1.009	-	1.0 ± 0.3		
NO Offset	1.2	mV	-20 to +150		
NO _x Offset	0.7	mV	-20 to 150		
Stability at Zero	0.1	PPB	< 0.2		
Stability at Span	0.2	PPB	< 2 ppb @ 400 ppb span gas		

Calibrated by :

Adul Dangklom
(Mr.Adul Dangklom)

Approved by :

Peera Detudom
(Mr.Peera Detudom)

NO-NO₂-NO_x AnalyzerEquipment : NO-NO₂-NO_x analyzer.

Model : 42i

Serial Number : CM13090047

Manufacturer : Thermo

Diagnostic test value

Parameter	Observed value		Unit	Nominal range
	Before	After		
Sample reading				
NO reading			ppb	
NO _x reading			ppb	
Range			ppb	50 to 1000 ppb
Averaging Time			Sec	10 to 300 Sec
Calibration Factors				
NO BKG. ppb			ppb	0 to 60
NO _x BKG. ppb			ppb	0 to 60
NO COEF.			-	1.0 ± 0.3
NO _x COEF.			-	1.0 ± 0.3
NO ₂ COEF.			-	1.0 ± 0.3
Instrument Controls				
Ozonator				On/Off
PMT Supply				On/Off
Auto/Manual Mode				NO/NO _x , NO, NO _x
Baud Rate			bps	1200 to 9600
Temp Compensation			-	On/Off
Pressure Compensation			-	On/Off
Screen Contrast			%	0 to 100
Service Mode			-	On/Off, Up to used
Diagnostics				
Voltages				
Motherboard voltages:				
3.3 Supply			Vdc	3.3 ± 1 Vdc
5.0 Supply			Vdc	5.0 ± 1 Vdc
15.0 Supply			Vdc	15.0 ± 1 Vdc
24.0 Supply			Vdc	24.0 ± 1 Vdc
-3.3 Supply			Vdc	-3.3 ± 1 Vdc
Interface board voltages:				
PMT Supply			Vdc	-400 to -1200 Vdc
3.3 Supply			Vdc	3.3 ± 1 Vdc
5.0 Supply			Vdc	5.0 ± 1 Vdc
15.0 Supply			Vdc	15.0 ± 1 Vdc
P15.0 Supply			Vdc	15.0 ± 1 Vdc
24.0 Supply			Vdc	24.0 ± 1 Vdc
-15.0 Supply			Vdc	-15.0 ± 1 Vdc
Temperatures				
Internal			°C	15 °C to 45 °C
Chamber			°C	50°C ± 2 °C
Cooler			°C	(-)3 °C ± 2 °C
Converter			°C	325 °C ± 5 °C
Converter Set			°C	325 °C
Pressure			mmHg	250 ± 100 mmHg
Flow			L/min	0.5 to 1.00 L/min

Note :



บริษัท คิว-ซี โซลูชันส์ จำกัด

7/409 ซอยวิภาวดีรังสิต 36 ถนนวิภาวดีรังสิต แขวงจตุจักร เขตจตุจักร กรุงเทพฯ 10900

โทรศัพท์ : (662) 939-5711 (12 Lines) โทรสาร : (662) 939-4207-8

Website <http://www.qshe.co.th> E-mail-address: info@qshe.co.th

SINGLE-POINT GAS CALIBRATION

NO_x, SO₂, CO Analyzer.

Equipment :	All analyzer.	Model :	42i, 43i,THC
Serial Number :	--	Manufacturer :	Thermo, Horiba

Standard gas concentration			Dilutor detail	
Sulfur Dioxide (SO ₂)	44.44	ppm	Manufacturer :	Thermo
Nitric Oxide (NO)	45.84	ppm	Model :	146i
Methane (CH ₄)	506.7	ppm	Serial number :	1201351404
Carbon Monoxide (CO)	4513	ppm		
Cylinder NO. :	CC507818			
Expiration Date :	13 Aug 2023			

BEFORE CALIBRATION RESULT

PARAMETER	ZERO			SPAN			JUDGEMENT
	IDEAL	ACTUAL	ERROR	IDEAL	ACTUAL	%ERROR	
NO (ppb)	0.00			400			
NO _x (ppb)	0.00			400			
SO ₂ (ppb)	0.00			400			
CH ₄ (ppm)	0.00			4.43			
THC(ppm)	0.00			4.43			

AFTER CALIBRATION RESULT

PARAMETER	ZERO			SPAN			JUDGEMENT
	IDEAL	ACTUAL	ERROR	IDEAL	ACTUAL	%ERROR	
NO (ppb)	0.00			400			
NO _x (ppb)	0.00			400			
SO ₂ (ppb)	0.00			400			
CH ₄ (ppm)	0.00			4.00			
THC(ppm)	0.00			4.00			

Remark:



บริษัท คิว-ชี โซลูชั่นส์ จำกัด

7/409 ซอยวิภาวดีรังสิต 36 ถนนวิภาวดีรังสิต แขวงจตุจักร เขตจตุจักร กรุงเทพฯ 10900

โทรศัพท์ : (662) 939-5711 (12 Lines) โทรสาร : (662) 939-4207-8

Website <http://www.qshe.co.th> E-mail-address: info@qshe.co.th

ภาพถ่ายการเข้าปฏิบัติงานตามแผนการบำรุงรักษา

Stations Mobile 3



Inside Station





CERTIFICATE No : 25M2254

REFERENCE No : 76365-1

PAGE : 1 OF 2

Certificate of Calibration

EQUIPMENT : DIGITAL BALANCE

MANUFACTURER : METTLER TOLEDO

MODEL : XS105DU

SERIAL No : 1126422905

ID No : BA05/50

CONDITION AS RECEIVED : USED ITEM

SUBMITTED BY : S.P.S. CONSULTING SERVICE CO., LTD.
7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN RD.,
JOMPOL, CHATUCHAK, BANGKOK 10900

CALIBRATED BY : ATSAWIN Y.

CALIBRATION DATE : 07-Mar-25

APPROVED BY : 
PONGSAK J.

ISSUED DATE : 13-Mar-25

RECEIVED DATE : 07-Mar-25

THIS CERTIFICATE MAY NOT BE REPRODUCED OTHER THAN IN FULL EXCEPT WITH THE PRIOR WRITTEN APPROVAL OF
QUALITY CALIBRATION CO., LTD.





CERTIFICATE No : 25M2254

PAGE : 2 OF 2

Calibration Report

EQUIPMENT : DIGITAL BALANCE MODEL : XS105DU
MANUFACTURER : METTLER TOLEDO S/N : 1126422905
ID No : BA05/50 RECEIVED DATE : 07-Mar-25
AIR PRESSURE : 1009mbar \pm 1mbar CALIBRATION DATE : 07-Mar-25
AMBIENT TEMPERATURE : 24°C \pm 1°C RELATIVE HUMIDITY : 54 %RH \pm 10 % RH

CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED BY ACCORDING TO UKAS LAB 14 EDITION 6:2019 BY USING KNOWN WEIGHT STANDARD WEIGHT. THE BALANCE WAS NOT ADJUSTED BEFORE CALIBRATION. THE BALANCE HAS NO ZERO TRACKING FUNCTION. REPEATABILITY WAS MEASURED BY USING 10 REPEATED MEASUREMENTS. LINEARITY WAS MEASURED COVERING 10 POINTS, EVENLY SPREAD OVER THE RANGE. THE INSTRUMENT WAS SET ZERO BEFORE PERFORMING THE LINEARITY TEST. OFF-CENTER LOADING WAS MEASURED BY USING STANDARD WEIGHTS PLACED ON THE PAN AND MOVED TO VARIOUS POSITIONS ON THE PAN.

2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) STANDARD WEIGHT SET	E2	QK-I-151	C02250116	28-Jan-27
2) STANDARD WEIGHT	E2	15843	C02250117	29-Jan-27

3. THE CERTIFICATE IS VALID FOR THE ITEM CALIBRATED AS SHOWN ON THE DATE AND PLACE OF CALIBRATION ONLY.

4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.

5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-

- NATIONAL INSTITUTE OF METROLOGY (THAILAND)

RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

1. ZERO SETTING FUNCTION : NORMAL

2. TARE FUNCTION : NORMAL

3. REPEATABILITY OF READING AT 120 g WAS 0.000055 g

4. DEPARTURE FROM NOMINAL VALUE/ LINEARITY

NOMINAL VALUE (g)	BALANCE READING (g)	CORRECTION (g)	UNCERTAINTY (\pm g)
0.00	0.00000	0.00000	0.000065
0.02	0.01999	0.00001	0.000065
0.10	0.10001	-0.00001	0.000066
0.20	0.20001	-0.00001	0.000066
0.50	0.50002	-0.00002	0.000065
1.00	1.00003	-0.00003	0.000066
2.00	2.00001	-0.00001	0.000067
5.00	5.00002	-0.00002	0.000068
10.00	10.00000	0.00000	0.000070
20.00	20.00004	-0.00004	0.000078
50.00	50.00000	0.00000	0.00013
100.00	100.0001	-0.0001	0.00019
120.00	120.0002	-0.0002	0.00022

5. OFF CENTER LOADING ERROR



POINT	READING (g)
1	50.0000
2	50.0000
3	50.0000
4	50.0000
5	50.0000
OFF-CENTER LOADING	0.0000

NOTE: THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA
THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR $k=2$, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT



ลำดับที่ 2

คุณภาพอากาศจากปล่อง



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72. Fax : (662) 513-4221. E-mail : sale@spscon.com.. www.spscon.com

Console Calibration Report

Calibration Method

Critical Orifices

Calibration Data

Console Data		Calibration Data		
No.	Serial No.	Date	y	DH _g (mmH ₂ O)
B01	1563	03/03/2025	1.003	49.40
B02	8002514	03/03/2025	1.004	49.57
B03	1503016	04/03/2025	0.999	49.93
B04	00006659	04/03/2025	0.996	49.88
B05	00007428	04/03/2025	1.007	49.14
R01	1561	05/03/2025	0.996	49.32
R02	8002513	04/03/2025	1.003	49.96
R03	1570	04/03/2025	0.998	50.08
R04	8002519	03/03/2025	0.997	49.53
R05	1503015	05/03/2025	1.005	50.25

Remark : Accept Value of y (test) is $0.97 < y < 1.03$

Accept Value of DH_g (test) is 46.7 ± 6.4 (mmH₂O)

Calibrated by :

Adul Dangklom
(Mr. Adul Dangklom)

Approved by :

Peera Detudom
(Mr. Peera Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด

S.P.S. CONSULTING SERVICE CO., LTD.

7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจตุจักร เขตจตุจักร กรุงเทพฯ 10900

7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900

Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

Pitot Tube Calibration Report

Calibration Method

Standard Pitot Tube

Calibration Data

Pitot Tube Data			Calibration Data		
No.	Type of Pitot	Coefficient of Standard Pitot	Date	Avg. of Cp (test)	
				Side A	Side B
B36	S	0.99	03/02/2025	0.84	0.83
B37	S	0.99	03/02/2025	0.85	0.84
B38	S	0.99	04/02/2025	0.84	0.85
B39	S	0.99	05/02/2025	0.84	0.83
B40	S	0.99	03/02/2025	0.84	0.84
B41	S	0.99	03/02/2025	0.84	0.84
B44	S	0.99	03/02/2025	0.85	0.84
B45	S	0.99	04/02/2025	0.84	0.83
B46	S	0.99	03/02/2025	0.84	0.84
B47	S	0.99	06/02/2025	0.84	0.85
B48	S	0.99	03/02/2025	0.84	0.84
B49	S	0.99	06/02/2025	0.85	0.84
B54	S	0.99	03/02/2025	0.84	0.84
B56	S	0.99	05/02/2025	0.84	0.84
B57	S	0.99	05/02/2025	0.85	0.84
B58	S	0.99	05/02/2025	0.84	0.85

Remark : Accept value of Cp (test) is 0.84 ± 0.01

Calibrated by :

Adul Dangklom
(Mr. Adul Dangklom)

Approved by :

Peera Detudom
(Mr. Peera Detudom)

CERTIFICATE OF CALIBRATION FOR

NOMENCLATURE : VACUUM GAUGE
MANUFACTURER : HI-LIGHT
MODEL / TYPE : N/A
SERIAL NO. : N/A[64-220066-2]
CLID. NO. : 212201113
JOB CONTROL NO. : 240730078440
CALIBRATION SERVICE : ☒ IN-LABORATORY ☐ ON-SITE

CUSTOMER : S.P.S. CONSULTING SERVICE CO., LTD.
7 SOI PHAHOLYOTHIN 24 ROAD., JOMPOL,
CHATUCHAK, BANGKOK 10900

DATE OF RECEIVED : 30 July 2024

DATE OF ISSUED : 02 August 2024

The report of calibration shall not be reproduced except in full without approval of the Calibration Laboratory Co., Ltd.

Calibrated By : Sittipong Pimdee
Calibration Engineer

Approved By : Mongkol Yotsoontorn
Authorized Signatory
02 August 2024



This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to the International System of Units (SI)

Certificate No. Q24078440

F3-011-05/12-23

page 1 of 3



@clccalibration



CALIBRATION LABORATORY Co., LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



REPORT OF CALIBRATION

FOR

NOMENCLATURE	:	VACUUM GAUGE
MANUFACTURER	:	HI-LIGHT
MODEL / TYPE	:	N/A
SERIAL NO.	:	N/A[64-220066-2]
DATE OF CALIBRATION	:	31 July 2024
DUE DATE OF CALIBRATION	:	31 July 2025

ENVIRONMENT CONDITIONS :

Temperature : $(23 \pm 2) ^\circ\text{C}$

Relative Humidity : $(55 \pm 10) \% \text{RH}$

PROCEDURE USED :

This instrument was calibrated under procedure No. **CLC-CPPP-05** according to **DKD-R 6-1** as calibration guidelines.

The calibration was performed by direct measurement with Document Process Calibrator and Pressure Module which maintained by the Calibration Laboratory Co., Ltd.

REFERENCE STANDARD USED :

Document Process Calibrator, Fluke Model 741B S/N. 8295020 with Pressure Module Model 700PD5 S/N. 89404505.

TRACEABILITY :

The measurements are traceable to International System of Units (SI), through National Institute of Metrology (Thailand).
Certificate No. MP-0040-24, Due Date 08 February 2025.

UNCERTAINTY :

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor of $k = 2$. It has been evaluated according to the "Calibration of Pressure Gauges (DKD-R 6-1)" which provides a level of confidence approximately 95%.

Certificate No. Q24078440

F3-011-05/12-23

page 2 of 3



@clccalibration

CONDITION OF CALIBRATION ITEM : RECEIVED IN GOOD OPERATIONAL CONDITION

MEASUREMENT RESULTS : (X) without adjustment () adjustment

The DUC was exercised by applying a known pressure from its zero to full scale 1 times. Then 2 series of known gauge pressure were applied. The STD reading were recorded and the means value were reported in the table below.

CALIBRATION DATA

CORRECTION OF PRESSURE

DUC Test point (inHg)	STD Reading (kPa)		Conversion to inHg		Correction (inHg)	
	Up	Down	Up	Down	Up	Down
0	0.000	0.000	0.0	0.0	0.0	0.0
-5	-16.591	-16.930	-4.9	-5.0	+0.1	0.0
-10	-33.521	-33.521	-9.9	-9.9	+0.1	+0.1
-15	-50.113	-50.113	-14.8	-14.8	+0.2	+0.2
-20	-66.704	-67.043	-19.7	-19.8	+0.3	+0.2
-25	-83.634	-83.973	-24.7	-24.8	+0.3	+0.2
-30	-100.564	-100.564	-29.7	-29.7	+0.3	+0.3

Uncertainty of measurement ± 0.2 inHg

Transmitting fluid : Air.

Technical Note. Conversion factor 1 kPa ; 0.2953003 inHg

Note. The Scope of Accredited ANAB Certificate No. ACDM-2814 Version 012 Page 43 of 67

This report is valid for the above stated instrument/s only.

End of Certificate

Certificate No. Q24078440

F3-011-05/12-23

page 3 of 3





บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

Personal Pump Calibration Report

Calibration Method : Dry Cal Primary Flowmeter

Model : Defender 510-H

S/N : 136164

Environmental Conditions

Temperature : 25 ± 3 °C
Pressure : 1010 ± 15 mmbar

Personal Pump Data				Calibration Data								
No.	Brand	Model	Serial No.	Date	Flow Rate (mL/min)						Value From Calibration Curve	
					Setting			Actual (Q std.)				
					1	2	3	1	2	3	y	R ²
B41	SKC	224-PCXR4	612669	03/04/2025	1,000	1,500	2,000	1,005	1,502	2,004	1.005x - 8.923	1.000
B42	SKC	224-PCXR4	626041	03/04/2025	1,000	1,500	2,000	1,004	1,501	2,008	1.009x - 13.856	1.000
B43	SKC	224-PCXR4	034636	01/04/2025	1,000	1,500	2,000	1,012	1,497	1,996	0.990x + 15.132	1.000
B44	SKC	224-PCXR8	529341	01/04/2025	1,000	1,500	2,000	1,011	1,511	2,008	1.002x - 0.860	0.999
B45	SKC	224-PCXR8	529594	04/04/2025	1,000	1,500	2,000	993	1,512	2,003	1.009x - 14.476	1.000
B46	SKC	224-PCXR8	566743	04/04/2025	1,000	1,500	2,000	1,008	1,508	2,008	1.000x - 0.100	0.999
B47	SKC	224-PCXR8	566747	04/04/2025	1,000	1,500	2,000	999	1,510	2,010	1.010x - 14.444	1.000
B48	SKC	224-PCXR8	566753	01/04/2025	1,000	1,500	2,000	1,010	1,506	2,006	0.999x + 2.782	1.000
B49	SKC	224-PCXR8	566780	04/04/2025	1,000	1,500	2,000	1,003	1,504	2,004	1.003x - 2.183	1.000
B50	SKC	224-PCXR8	500400	04/04/2025	1,000	1,500	2,000	1,002	1,493	1,995	0.994x + 5.841	1.000
B51	SKC	224-PCXR8	500363	04/04/2025	1,000	1,500	2,000	998	1,511	2,011	1.013x - 19.465	0.999
B52	SKC	224-PCXR8	093186	02/04/2025	1,000	1,500	2,000	997	1,505	2,006	1.008x - 12.641	1.000
B53	SKC	224-PCXR8	707670	02/04/2025	1,000	1,500	2,000	1,004	1,503	2,007	1.007x - 7.992	1.000
B54	SKC	224-PCXR3	509821	02/04/2025	1,000	1,500	2,000	1,005	1,504	2,008	1.010x - 15.060	0.999
B55	SKC	224-PCXR3	510710	02/04/2025	1,000	1,500	2,000	1,001	1,495	1,997	0.996x + 5.073	1.000
B56	SKC	224-PCXR3	511450	02/04/2025	1,000	1,500	2,000	1,005	1,494	1,996	0.991x - 13.385	1.000
B57	SKC	224-PCXR3	510798	03/04/2025	1,000	1,500	2,000	997	1,511	2,009	1.014x - 21.540	0.999
B58	SKC	224-PCXR3	509852	03/04/2025	1,000	1,500	2,000	1,006	1,493	2,002	1.001x - 4.094	1.000
B59	SKC	224-PCXR3	509862	03/04/2025	1,000	1,500	2,000	995	1,502	2,003	1.012x - 21.564	1.000
B60	SKC	224-PCXR3	512655	03/04/2025	1,000	1,500	2,000	998	1,507	2,004	1.010x - 18.510	0.999
B61	SKC	224-PCXR3	503915	03/04/2025	1,000	1,500	2,000	997	1,499	2,001	1.002x - 4.374	1.000
B62	SKC	224-PCXR3	505975	01/04/2025	1,000	1,500	2,000	1,002	1,503	2,005	1.008x - 11.138	1.000
B63	SKC	224-PCXR3	511432	04/04/2025	1,000	1,500	2,000	998	1,502	1,996	0.996x + 3.970	1.000
B64	SKC	224-PCXR3	508302	04/04/2025	1,000	1,500	2,000	1,005	1,509	2,008	1.009x - 10.402	1.000
B65	SKC	224-PCXR3	508310	04/04/2025	1,000	1,500	2,000	1,004	1,503	2,007	1.010x - 14.088	1.000
B66	SKC	224-PCXR3	509861	04/04/2025	1,000	1,500	2,000	1,003	1,504	2,010	1.008x - 12.369	1.000
B67	SKC	224-PCXR3	506295	04/04/2025	1,000	1,500	2,000	1,002	1,498	2,004	0.998x + 4.290	1.000
B68	SKC	224-PCXR3	505872	04/04/2025	1,000	1,500	2,000	999	1,504	1,998	1.000x + 0.436	1.000
B69	SKC	224-PCXR3	508375	02/04/2025	1,000	1,500	2,000	1,004	1,498	2,002	0.996x + 5.501	1.000
B70	SKC	224-PCXR3	510623	02/04/2025	1,000	1,500	2,000	996	1,497	2,005	1.005x - 8.735	1.000
B71	SKC	224-PCXR3	508367	02/04/2025	1,000	1,500	2,000	1,013	1,505	2,009	1.000x + 3.294	0.999
B72	SKC	224-PCXR3	505977	02/04/2025	1,000	1,500	2,000	997	1,494	2,003	1.006x - 11.350	1.000
B73	SKC	224-PCXR3	512606	01/04/2025	1,000	1,500	2,000	1,010	1,507	2,004	0.998x + 5.129	1.000
B74	SKC	224-PCXR3	505993	01/04/2025	1,000	1,500	2,000	998	1,499	2,010	1.009x - 11.942	1.000
B75	SKC	224-PCXR3	509820	01/04/2025	1,000	1,500	2,000	995	1,511	2,004	1.011x - 18.966	0.999
B76	SKC	224-PCXR3	509811	01/04/2025	1,000	1,500	2,000	998	1,504	2,010	1.012x - 20.993	0.999
B77	SKC	224-PCXR3	508301	03/04/2025	1,000	1,500	2,000	1,007	1,509	2,008	1.001x + 3.750	1.000
B78	SKC	224-PCXR3	510677	04/04/2025	1,000	1,500	2,000	998	1,508	2,001	1.003x - 3.278	1.000
B79	SKC	224-PCXR3	510920	04/04/2025	1,000	1,500	2,000	1,001	1,501	1,994	0.999x - 1.819	1.000

Calibrated by :

Adul Dangklom
(Mr. Adul Dangklom)

Approved by :

(Mr. Peera Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
 7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
 7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
 Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

Rotameter Calibration Report (For Personal Pump High Flow Adjust)

Calibration Method : Dry Cal Primary Flowmeter

Model : Defender 510-H

S/N : 136164

Calibration Data

Rotameter Data			Calibration Data								
No.	Brand	Model	Date	Flow Rate (mL/min)						Value From Calibration Curve	
				Flow Rate (Reading)			Actual (Q std.)				
				1	2	3	1	2	3	y	R ²
H-R01	Dwyer	VFB-65	02/04/2025	500	1,000	2,000	499.6	998.8	2004.8	1.001x - 3.678	1.000
H-R02	Dwyer	VFB-65	02/04/2025	500	1,000	2,000	501.7	997.1	1991.5	0.998x + 0.386	0.999
H-R03	Dwyer	VFB-65	01/04/2025	500	1,000	2,000	499.8	999.7	1992.8	1.000x + 1.316	1.000
H-R04	Dwyer	VFB-65	04/04/2025	500	1,000	2,000	500.2	999.4	1989.2	0.999x + 1.870	0.999
H-R05	Dwyer	VFB-65	04/04/2025	500	1,000	2,000	499.9	1000.8	1994.5	1.000x + 0.815	1.000
H-R06	Dwyer	VFB-65	03/04/2025	500	1,000	2,000	500.5	1001.3	1990.7	0.997x + 4.894	0.999

Calibrated by :

Adul Dangklom
 (Mr.Adul Dangklom)

Approved by :

Mr. Peera Detudom
 (Mr. Peera Detudom)



CERTIFICATE No : 25M2254

REFERENCE No : 76365-1

PAGE : 1 OF 2

Certificate of Calibration

EQUIPMENT : DIGITAL BALANCE

MANUFACTURER : METTLER TOLEDO

MODEL : XS105DU

SERIAL No : 1126422905

ID No : BA05/50

CONDITION AS RECEIVED : USED ITEM

SUBMITTED BY : S.P.S. CONSULTING SERVICE CO., LTD.
7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN RD.,
JOMPOL, CHATUCHAK, BANGKOK 10900

CALIBRATED BY : ATSAWIN Y.

CALIBRATION DATE : 07-Mar-25

APPROVED BY : 
PONGSAK J.

ISSUED DATE : 13-Mar-25

RECEIVED DATE : 07-Mar-25

THIS CERTIFICATE MAY NOT BE REPRODUCED OTHER THAN IN FULL EXCEPT WITH THE PRIOR WRITTEN APPROVAL OF
QUALITY CALIBRATION CO., LTD.





CERTIFICATE No : 25M2254

PAGE : 2 OF 2

Calibration Report

EQUIPMENT : DIGITAL BALANCE MODEL : XS105DU
MANUFACTURER : METTLER TOLEDO S/N : 1126422905
ID No : BA05/50 RECEIVED DATE : 07-Mar-25
AIR PRESSURE : 1009mbar \pm 1mbar CALIBRATION DATE : 07-Mar-25
AMBIENT TEMPERATURE : 24° C \pm 1° C RELATIVE HUMIDITY : 54 %RH \pm 10 % RH

CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED BY ACCORDING TO UKAS LAB 14 EDITION 6:2019 BY USING KNOWN WEIGHT STANDARD WEIGHT. THE BALANCE WAS NOT ADJUSTED BEFORE CALIBRATION. THE BALANCE HAS NO ZERO TRACKING FUNCTION. REPEATABILITY WAS MEASURED BY USING 10 REPEATED MEASUREMENTS. LINEARITY WAS MEASURED COVERING 10 POINTS, EVENLY SPREAD OVER THE RANGE. THE INSTRUMENT WAS SET ZERO BEFORE PERFORMING THE LINEARITY TEST. OFF-CENTER LOADING WAS MEASURED BY USING STANDARD WEIGHTS PLACED ON THE PAN AND MOVED TO VARIOUS POSITIONS ON THE PAN.

2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) STANDARD WEIGHT SET	E2	QK-I-151	C02250116	28-Jan-27
2) STANDARD WEIGHT	E2	15843	C02250117	29-Jan-27

3. THE CERTIFICATE IS VALID FOR THE ITEM CALIBRATED AS SHOWN ON THE DATE AND PLACE OF CALIBRATION ONLY.

4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.

5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-

- NATIONAL INSTITUTE OF METROLOGY (THAILAND)

RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

1. ZERO SETTING FUNCTION : NORMAL

2. TARE FUNCTION : NORMAL

3. REPEATABILITY OF READING AT 120 g WAS 0.000055 g

4. DEPARTURE FROM NOMINAL VALUE/ LINEARITY

NOMINAL VALUE (g)	BALANCE READING (g)	CORRECTION (g)	UNCERTAINTY (\pm g)
0.00	0.00000	0.00000	0.000065
0.02	0.01999	0.00001	0.000065
0.10	0.10001	-0.00001	0.000066
0.20	0.20001	-0.00001	0.000066
0.50	0.50002	-0.00002	0.000065
1.00	1.00003	-0.00003	0.000066
2.00	2.00001	-0.00001	0.000067
5.00	5.00002	-0.00002	0.000068
10.00	10.00000	0.00000	0.000070
20.00	20.00004	-0.00004	0.000078
50.00	50.00000	0.00000	0.00013
100.00	100.0001	-0.0001	0.00019
120.00	120.0002	-0.0002	0.00022

5. OFF CENTER LOADING ERROR



POINT	READING (g)
1	50.0000
2	50.0000
3	50.0000
4	50.0000
5	50.0000
OFF-CENTER LOADING	0.0000

NOTE: THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA
THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR $k=2$, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT



Cert. No. : SP24020

Pages 1 of 3

Calibration Certificate

Equipment : UV-VIS SPECTROPHOTOMETER
Manufacturer : PERKINELMER
Model : LAMBDA 25
Serial No.: 501S14123010
ID No.: SP03/58
Calibration Mode : WAVELENGTH ACCURACY
PHOTOMETRIC ACCURACY

Condition As Found : GOOD

Customer : S.P.S. CONSULTING SERVICE CO., LTD.
7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN ROAD,
CHOMPHON, CHATUCHAK,
BANGKOK 10900, THAILAND.

Location : WET CHEMISTRY LABORATORY IV

Ambient Temperature : (28.1 ± 5) °C
Relative Humidity : (47.2 ± 25) %

Received Date : 27 AUGUST 2024
Calibration Date : 27 AUGUST 2024
Date of Issue : 27 AUGUST 2024

Calibrated by : Nathakorn Pisutpaisan

Approved by :


(Thanakul Petchurai)

SITHIPORN ASSOCIATES CO., LTD.

CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Banglumru, Bangplud, Bangkok, 10700 Thailand
Tel. +66 2433 8331 Email : calibration@sithiporn.com

SITHIPORN
associates



Cert. No. : SP24020

Job No. : VC67SP0013

Pages : 2 of 3

Calibration Method :

This instrument was calibrated by using on-site calibration procedure In-house method : CP-SP-01

The calibration procedure to direct measurement wavelength accuracy by using wavelength standard solution, Photometric accuracy by using absorbance standard filter and absorbance standard solution

The calibration procedure used was based on ASTM E275-01, ASTM E925-02

Condition of this result of calibration :

1. Certified reference materials

Material	Ref. type	Cell serial No.	Cert. No.	Due Date
Holmium liquid	RM-HL	29706	106864	01/11/2024
Didymium liquid	RM-DL	28912	106905	02/11/2024
Neutral density filter	RM-1N2N3N	13877	106918	03/11/2024
Potassium dichromate solutions	RM-0204060810	14204	106902	02/11/2024
Potassium Iodide solution	-	KI-0701-001	CI-0185-24	14/05/2026

2. This result of calibration was found accurate as shown on date and place of calibration only.

3. This certificate is traceable to the international system of unit maintained at :

3.1 The UK National Physical Laboratory (NPL)

3.2 The National Institute of Standards and Technology, NIST.

Result of calibration : Wavelength Accuracy

(Without adjustment)

Material	Certified Values of Reference Material (nm)	UUC* Reading (nm)	Error (nm)	Uncertainty ± (nm)	k Factor
RM-HL	278.13	278.3	0.17	0.16	2.00
	361.25	361.4	0.15	0.16	2.00
	467.82	467.7	-0.12	0.16	2.00
	536.56	536.5	-0.06	0.16	2.00
	640.50	640.4	-0.10	0.16	2.00
RM-DL	740.09	739.9	-0.19	0.16	2.00
	864.94	865.2	0.26	0.16	2.00

UUC* = Unit Under Calibration

G. Petch

SITHIPORN ASSOCIATES CO., LTD.

CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbunru, Bangplud, Bangkok, 10700 Thailand
Tel. +66 2433 8331 Email : calibration@sithiporn.com

SITHIPORN
associates



Cert. No. : SP24020

Job No. : VC67SP0013

Pages : 3 of 3

Result of calibration : Photometric Accuracy

(Without adjustment)

Material	Wavelength (nm)	Filter S/N	Nominal Absorbance (A)	Certified Absorbance (A)	UUC* Reading Absorbance (A)	Error (A)	Uncertainty ± (A)	k Factor
Neutral Density glass filter	440.0	29360	1.0	1.0517	1.0550	0.0033	0.0029	2.00
		29914	0.7	0.7445	0.7460	0.0015	0.0029	2.00
		29381	0.5	0.5416	0.5431	0.0015	0.0030	2.00
	546.1	29360	1.0	0.9821	0.9820	-0.0001	0.0028	2.00
		29914	0.7	0.6961	0.6958	-0.0003	0.0028	2.00
		29381	0.5	0.5073	0.5080	0.0007	0.0029	2.00
	590.0	29360	1.0	1.0222	1.0210	-0.0012	0.0028	2.00
		29914	0.7	0.7237	0.7221	-0.0016	0.0029	2.00
		29381	0.5	0.5361	0.5361	0.0000	0.0031	2.00
	635.0	29360	1.0	0.9753	0.9745	-0.0008	0.0028	2.00
		29914	0.7	0.6910	0.6900	-0.0010	0.0029	2.00
		29381	0.5	0.5211	0.5210	-0.0001	0.0032	2.00
Material	Wavelength (nm)	Solution (mg/l)	Certified Absorbance (A)	UUC* Reading Absorbance (A)	Error (A)	Uncertainty ± (A)	k Factor	
RM-0204060810	235.0	20	0.2422	0.2418	-0.0004	0.0101	2.00	
		40	0.4866	0.4852	-0.0014	0.0115	2.00	
		60	0.7414	0.7389	-0.0025	0.0067	2.00	
		80	0.9858	0.9842	-0.0016	0.0093	2.00	
		100	1.2442	1.2414	-0.0028	0.0086	2.00	

UUC* = Unit Under Calibration

Condition of this result of calibration : Spectrophotometer PERKINELMER Model Lambda 25 S/N 501S14123010

Resolution of Wavelength Mode 0.1 nm

Resolution of Photometric Mode 0.0001 A

Parameter Setting

Measurement Mode Wavelength, Absorbance

Wavelength Scan 1100 nm-190 nm

Scanning Speed 7.5 nm/min

Data Pitch 0.1 nm

Band width(Wavelength) 1.0 nm

Band width(Vis) 1.0 nm

Band width(Uv) 1.0 nm

Stray Light** UUC* Reading at 220 nm

Transmission T(%)	Absorbance(A)
0.0117	3.8659

**Specific Acceptance :

Transmission \leq 1.0 T(%), Absorbance \geq 2.0 A

**Stray light not TISI Accredited

The reported uncertainty is based on a standard uncertainty multiplied by a coverage factor k , providing a level of confidence of approximately 95%

End of Calibration Certificate

T. Ketch



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

Calibration Report					
Non-Dispersive Infrared CO Analyzer					
Date :	01 April 2025	Brand :	API	Model :	300E
No.	CO-R02			Serial No.	171-S
Calibrator (Dilution System)					
Brand : Teledyne			Model : 700E		
Last Cal. Date : 28 October 2024			Serial No. : 201-S		
Reference Standard Gas					
Standard Gas : Carbon Monoxide (CO)			Cylinder No. : D711839		
Certified Date : 14 March 2024		Expired Date : 14 March 2032		Cylinder Conc. : 4,580 ppm	
Calibrating Condition					
Pressure : 1011 mmbar		Temp. : 24.6 °C		% RH : 50	
Calibration Setting					
Span	Initial Reading (Before Adj.), PPM			Final Reading (After Adj.), PPM	
Set Point	Expected Concentration	Analyzer Response		%Dif	
Zero	0	-0.10		-	
CO Span	40.00	39.95		-0.125	
API Model 300E CO Analyzer Check List					
Parameter	Observed Value	Units	Nominal Range		
Range	50	PPM	0-1000 ppm		
Stability	0.10	PPM	< 1 ppm With Zero Air		
CO Measure	4013.5	mV	2500-4800 mV		
CO Reference	3947.2	mV	2500-4800 mV		
Measure/Reference Ratio	1.179	-	1.1-1.3 W/Zero Air		
Sample Pressure	28.5	In-Hg-A	~2" < Ambient Absolute Pressure		
Sample Flow	808	CC/Min	800 ± 10%		
Sample Temperature	48.5	°C	48 ± 4		
Bench Temperature	48.2	°C	48 ± 2		
Wheel Temperature	68.3	°C	68 ± 2		
Box Temperature	30.6	°C	Ambient Temp + 7 ± 10		
Photo-Drive	3036.9	mV	250 mV to 4750 mV		
Slope	1.017	-	1.0 ± 0.3		
Offset	0.2	-	0 ± 0.3		

Calibrated by : Adul Dangklom
(Mr. Adul Dangklom)

Approved by : Peera Detudom
(Mr. Peera Detudom)

ลำดับที่ 3

ระดับเสียงในบรรยากาศทั่วไป



THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-68/0220

MTC No. EEL. BP. 45/0268

CALIBRATION CERTIFICATE

Submitted by : S.P.S.Consulting Service Co.,Ltd.

Address : 7 Soi Phaholyothin 24, Phaholyothin Road, Jompol, Chatuchak, Bangkok 10900.

Calibrated at : Electrical and Electronic Standards Laboratory, Industrial Metrology and Testing Service Centre.
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Rd., Muang, Samutprakan 10280.

Instrument Calibrated :

Description : Acoustic Calibrator

Manufacturer : Cirrus Research plc

Model : CR:515

Serial No. : 92002

Ambient Environment

Temperature : $(23 \pm 3) ^\circ\text{C}$

Relative Humidity : $(50 \pm 15) \%$

Ambient Pressure : $(101.325 \pm 1.500) \text{ kPa}$

- Standards used :
1. Digital Function Synthesizer NF Electronic DF-193A S/N 122037.
 2. Measuring Amplifier Bruel&Kjaer 2636 S/N 1537484.
 3. Programmable Attenuator Tamagawa TPA-303A S/N OF 2214.
 4. Digital Multimeter Agilent 34401A S/N MY44005560.
 5. Pressure Transmitter Vaisala PTB202AD S/N T0650001.
 6. Audio Analyzer Panasonic VP-7722A S/N 041477D122.
 7. Condenser Microphone B&K 4180 S/N 2889871.

Calibration Procedure: CP-102-04 based on IEC 60942-2003; The sound pressure level generated by sound calibrator under test shall be measured by standard microphone using an insert voltage technique.

This instrument has been calibrated against standards maintained at Electrical and Electronic Standards Laboratory (EEL), which are traceable to the International System of Units through the National Institute of Metrology (Thailand).

The information on actual reading is attached herewith and the uncertainty limits quoted refer to the measured values only.

Date of Receipt : 19 Feb. 2025

Date of Calibration : 21 Feb. 2025

1 / 2
W

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.5

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9009

Office/Laboratory
668 Mu 2 Tambon Bangpoomai, Amphoe Muang Samutprakan,
Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtc@tistr.or.th Website : www.tistr.or.th

Office
196 Phahonyothin Road, Ladyao, Chatuchak,
Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827

THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-68/0220

MTC No. EEL. BP. 45/0268

The reported expanded uncertainty is based upon a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%.

Nominal Output of Unit Under Test = 94 dB re 20 μ Pa at 1000 Hz

Acoustic Output in dB re 20 μ Pa, Corrected to Reference Conditions: 101.325 kPa, 23.0 °C and 50 %RH.

1. Sound Pressure Level

Standard Microphone Type	Measured Sound Pressure Level (dB)	Deviated value (dB)	Uncertainty (dB)	Tolerance limit IEC60942:2003 Class 1
1/2 inch Bruel&Kjaer 4180	93.98	-0.02	± 0.10	± 0.40 dB

2. Frequency

Standard Microphone Type	Measured Frequency (Hz)	Deviated value (Hz)	Uncertainty (Hz)	Tolerance limit IEC60942:2003 Class 1
1/2 inch Bruel&Kjaer 4180	1000.1	0.1	± 1.5	$\pm 1.0\%$

3. Total Distortion

Standard Microphone Type	Measured Total Distortion (%)	Uncertainty (%)	Tolerance limit IEC60942:2003 Class 1
1/2 inch Bruel&Kjaer 4180	0.65	± 0.50	$\pm 3.0\%$

Note : 1. No adjustment.

2. The calibrator pressure correction was not included.

3. The microphone volume correction was not included.

Calibrated by :


.....
(Mr. Weerachai Deechaiyae)

Approved by :



.....
f (Mr. Prawate Kluaypa)
Director

Date of Calibration : 21 Feb. 2025

Date of Issue : 24 Feb. 2025

Electrical and Electronic Standards Laboratory
Industrial Metrology and Testing Service Centre

Ref : 2011268021900739002

End of Certificate

2 / 2

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BLMTC.002 Rev.5

Head Office

35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9009

Office/Laboratory

668 Mu 2 Tambon Bangpoomai, Amphoe Muang Samutprakan,
Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtc@tistr.or.th Website : www.tistr.or.th

Office

196 Phahonyothin Road, Ladyao, Chatuchak,
Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจตุจักร เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72 Fax : (662) 513-4221 E-mail : sale@spscon.com, www.spscon.com

Noise R_279/25

Sound Level Meter Calibration Report

Acoustic Calibrator Data

Brand	CIRRUS	Number	AC-CR01/63
Model	CR515	Serial No.	92002
Calibration Range	94 dB, 1000 Hz	Last Calibration	21 February 2025
		Due Date	21 February 2026

Calibration Data

Sound Level Meter Data				Calibration Data		
SLM No.	Brand	Model	Serial No.	Date	Actual Reading [dB]	
					Before Adjustment	After Adjustment
CR-B02	Cirrus	CR161B	G301157	28 April 2025	94.0	94.0
CR-B04	Cirrus	CR161B	G301404	28 April 2025	94.0	94.0
CR-B05	Cirrus	CR161B	G301134	28 April 2025	94.1	94.0
CR-B06	Cirrus	CR161B	G301151	28 April 2025	94.0	94.0
CR-B07	Cirrus	CR161B	G301167	28 April 2025	94.0	94.0
CR-B08	Cirrus	CR161B	G301397	28 April 2025	94.0	94.0
CR-B09	Cirrus	CR161B	G301401	28 April 2025	94.0	94.0
CR-B10	Cirrus	CR161B	G301407	28 April 2025	94.0	94.0
Acoustic Certified Value : Thailand Institute of Scientific and Technological Research (TISTR)					93.98 ± 0.10 dB	

Calibrated by :

Adul Dangklom
(Mr. Adul Dangklom)

Approved by :

Peera Detudom
(Mr. Peera Detudom)

ลำดับที่ 4

ระดับเสียงในที่ทำงาน และระดับเสียงบริเวณอุปกรณ์ที่มีระดับเสียงเกิน 85 เดซิเบล (เอ)



THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-68/0220

MTC No. EEL. BP. 44/0268

CALIBRATION CERTIFICATE

Submitted by : S.P.S.Consulting Service Co.,Ltd.

Address : 7 Soi Phaholyothin 24, Phaholyothin Road, Jompol, Chatuchak, Bangkok 10900.

Calibrated at : Electrical and Electronic Standards Laboratory, Industrial Metrology and Testing Service Centre.
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Rd., Muang, Samutprakan 10280.

Instrument Calibrated :

Description : Sound Calibrator

Manufacturer : ACO

Model : 2127

Serial No. : 130006

Ambient Environment

Temperature : $(23 \pm 3) ^\circ\text{C}$

Relative Humidity : $(50 \pm 15) \%$

Ambient Pressure : $(101.325 \pm 1.500) \text{ kPa}$

- Standards used :
1. Digital Function Synthesizer NF Electronic DF-193A S/N 122037.
 2. Measuring Amplifier Bruel&Kjaer 2636 S/N 1537484.
 3. Programmable Attenuator Tamagawa TPA-303A S/N OF 2214.
 4. Digital Multimeter Agilent 34401A S/N MY44005560.
 5. Pressure Transmitter Vaisala PTB202AD S/N T0650001.
 6. Audio Analyzer Panasonic VP-7722A S/N 041477D122.
 7. Condenser Microphone B&K 4180 S/N 2889871.

Calibration Procedure: CP-102-04 based on IEC 60942-2003; The sound pressure level generated by sound calibrator under test shall be measured by standard microphone using an insert voltage technique.

This instrument has been calibrated against standards maintained at Electrical and Electronic Standards Laboratory (EEL), which are traceable to the International System of Units through the National Institute of Metrology (Thailand).

The information on actual reading is attached herewith and the uncertainty limits quoted refer to the measured values only.

Date of Receipt : 19 Feb. 2025

Date of Calibration : 21 Feb. 2025

1 / 2
W

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.5

Head Office

35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9009

Office/Laboratory

668 Mu 2 Tambon Bangpoomai, Amphoe Muang Samutprakan,
Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtc@tistr.or.th Website : www.tistr.or.th

Office

196 Phahonyothin Road, Ladyao, Chatuchak,
Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827

THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-68/0220

MTC No. EEL. BP. 44/0268

The reported expanded uncertainty is based upon a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%.

Nominal Output of Unit Under Test = 94 dB re 20 μ Pa at 1000 Hz

Acoustic Output in dB re 20 μ Pa, Corrected to Reference Conditions: 101.325 kPa, 23.0 °C and 50 %RH.

1. Sound Pressure Level

Standard Microphone Type	Measured Sound Pressure Level (dB)	Deviated value (dB)	Uncertainty (dB)	Tolerance limit IEC60942:2003 Class 1
1/2 inch Bruel&Kjaer 4180	93.81	-0.19	± 0.10	± 0.40 dB

2. Frequency

Standard Microphone Type	Measured Frequency (Hz)	Deviated value (Hz)	Uncertainty (Hz)	Tolerance limit IEC60942:2003 Class 1
1/2 inch Bruel&Kjaer 4180	999.9	-0.1	± 1.5	$\pm 1.0\%$

3. Total Distortion

Standard Microphone Type	Measured Total Distortion (%)	Uncertainty (%)	Tolerance limit IEC60942:2003 Class 1
1/2 inch Bruel&Kjaer 4180	0.95	± 0.50	$\pm 3.0\%$

Note : 1. No adjustment.

2. The calibrator pressure correction was not included.

3. The microphone volume correction was not included.

Calibrated by :


(Mr. Weerachai Deechaiyae)

Approved by :


(Mr. Prawate Khuaypa)
Director

Date of Calibration : 21 Feb. 2025

Date of Issue : 24 Feb. 2025

Electrical and Electronic Standards Laboratory
Industrial Metrology and Testing Service Centre

Ref : 2011268021900739001

End of Certificate

2 / 2

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.5

Head Office

35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9009

Office/Laboratory

668 Mu 2 Tambon Bangpoornai, Amphoe Muang Samutprakan,
Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtc@tistr.or.th Website : www.tistr.or.th

Office

196 Phahonyothin Road, Ladyao, Chatuchak,
Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827



THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-67/0562

MTC No. EEL. BP. 71/0767

CALIBRATION CERTIFICATE

Submitted by : S.P.S Consulting Services Co.,Ltd.

Address : 7 Soi Phaholyothin 24, Phaholyothin Road, Jompol, Chatuchak, Bangkok 10900.

Calibrated at : Electrical and Electronic Standards Laboratory, Industrial Metrology and Testing Service Centre.
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Rd., Muang, Samutprakan 10280.

Instrument Calibrated :

Description : Sound Calibrator

Manufacturer : SVANTEK

Model : SV34

Serial No. : 33137

Ambient Environment

Temperature : $(23 \pm 3) ^\circ\text{C}$

Relative Humidity : $(50 \pm 15) \%$

Ambient Pressure : $(101.325 \pm 1.500) \text{ kPa}$

- Standards used :
1. Digital Function Synthesizer NF Electronic DF-193A S/N 122037.
 2. Measuring Amplifier Briel&Kjaer 2636 S/N 1537484.
 3. Programmable Attenuator Tamagawa TPA-303A S/N OF 2214.
 4. Digital Multimeter Agilent 34401A S/N MY44005560.
 5. Pressure Transmitter Vaisala PTB202AD S/N T0650001.
 6. Audio Analyzer Panasonic VP-7722A S/N 041477D122.
 7. Condenser Microphone Briel&Kjaer 4180 S/N 2633526.

Calibration Procedure: CP-102-04 based on IEC 60942-2003; The sound pressure level generated by sound calibrator under test shall be measured by standard microphone using an insert voltage technique.

This instrument has been calibrated against standards maintained at Electrical and Electronic Standards Laboratory (EEL), which are traceable to the International System of Units through the National Institute of Metrology (Thailand).

The information on actual reading is attached herewith and the uncertainty limits quoted refer to the measured values only.

Date of Receipt : 31 Jul. 2024

Date of Calibration : 6 Aug. 2024

1 / 2

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.5

Head Office

35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9009

Office/Laboratory

668 Mu 2 Tambon Bangpoomai, Amphoe Muang Samutprakan,
Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtc@tistr.or.th Website : www.tistr.or.th

Office

196 Phahonyothin Road, Ladyao, Chatuchak,
Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827

THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-67/0562

MTC No. EEL. BP. 71/0767

The reported expanded uncertainty is based upon a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%.

Nominal Output of Unit Under Test = 114 dB re 20 μ Pa at 1000 Hz

Acoustic Output in dB re 20 μ Pa, Corrected to Reference Conditions: 101.325 kPa, 23.0 °C and 50 %RH.

1. Sound Pressure Level

Standard Microphone Type	Measured Sound Pressure Level (dB)	Deviated value (dB)	Uncertainty (dB)	Tolerance limit IEC60942:2003 Class 2
1/2 inch Bruel&Kjaer 4180	113.50	-0.50	± 0.10	± 0.75 dB

2. Frequency

Standard Microphone Type	Measured Frequency (Hz)	Deviated value (Hz)	Uncertainty (Hz)	Tolerance limit IEC60942:2003 Class 2
1/2 inch Bruel&Kjaer 4180	1000.0	0.0	± 1.5	$\pm 2.0\%$

3. Total Distortion


Standard Microphone Type	Measured Total Distortion (%)	Uncertainty (%)	Tolerance limit IEC60942:2003 Class 2
1/2 inch Bruel&Kjaer 4180	0.48	± 0.50	$\pm 4.0\%$

Note : 1. No adjustment.

2. The calibrator pressure correction was not included.

3. The microphone volume correction was not included.

Calibrated by :


.....
(Mr. Weerachai Deechaiyae)

Approved by :


.....
(Mr. Prawate Kluaypa)

Director

Electrical and Electronic Standards Laboratory

Industrial Metrology and Testing Service Centre

Date of Calibration : 6 Aug. 2024

Date of Issue : 7 Aug. 2024

Ref : 2011267073102836002

End of Certificate

2 / 2

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.5

Head Office

35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9009

Office/Laboratory

668 Mu 2 Tambon Bangpoomai, Amphoe Muang Samutprakan,
Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtc@tistr.or.th Website : www.tistr.or.th

Office

196 Phahonyothin Road, Ladyao, Chatuchak,
Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com., www.spscon.com

Noise R_213/25

Sound Level Meter Calibration Report

Acoustic Calibrator Data

Brand	ACO	Number	AC 03/56
Model	2127	Serial No.	130006
Calibration Range	94 dB, 1000 Hz	Last Calibration	21 February 2025
		Due Date	21 February 2026

Calibration Data

Sound Level Meter Data				Calibration Data		
SLM No.	Brand	Model	Serial No.	Date	Actual Reading [dB]	
					Before Adjustment	After Adjustment
ACO-B18	ACO	6236	00172048	07 April 2025	93.9	93.9
Acoustic Certified Value : Thailand Institute of Scientific and Technological Research (TISTR)					93.81 ± 0.10 dB	

Calibrated by :

Adul Dangklom
(Mr. Adul Dangklom)

Approved by :

Peera Detudom
(Mr. Peera Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด

S.P.S. CONSULTING SERVICE CO., LTD.

7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900

7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900

Tel : (662) 939-4370-72 Fax : (662) 513-4221 E-mail : sale@spscon.com, www.spscon.com

Noise R_050/25

Sound Level Meter Calibration Report

Acoustic Calibrator Data

Brand	ACO	Number	AC 03/56
Model	2127	Serial No.	130006
Calibration Range	94 dB, 1000 Hz	Last Calibration	04 March 2024
		Due Date	04 March 2025

Calibration Data

Sound Level Meter Data				Calibration Data		
SLM No.	Brand	Model	Serial No.	Date	Actual Reading [dB]	
					Before Adjustment	After Adjustment
ACO-R52	ACO	6236	00192064	20 January 2025	93.9	93.9
Acoustic Certified Value : Thailand Institute of Scientific and Technological Research (TISTR)					93.85 ± 0.10 dB	

Calibrated by :

Adul Dangklom
(Mr. Adul Dangklom)

Approved by :

Peera Detudom
(Mr. Peera Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

Noise Dose R_043/25

Noise Dose Meter Calibration Report

Acoustic Calibrator Data

Brand	SVANTEK	Number	SV 01/60
Model	SV34	Serial No.	33137
Calibration Range	114 dB, 1000 Hz	Last Calibration	06 August 2024
		Due Date	06 August 2025

Calibration Data

Sound Level Meter Data				Calibration Data		
SLM No.	Brand	Model	Serial No.	Date	Actual Reading [dB]	
					Before Adjustment	After Adjustment
NMD-B01	SVANTEK	SV-104IS	80840	19 January 2025	113.5	113.5
NMD-B02	SVANTEK	SV-104IS	80842	19 January 2025	113.6	113.5
NMD-B03	SVANTEK	SV-104IS	80852	19 January 2025	113.5	113.5
NMD-B04	SVANTEK	SV-104IS	80854	19 January 2025	113.5	113.5
NMD-B05	SVANTEK	SV-104IS	80856	19 January 2025	113.6	113.5
NMD-B06	SVANTEK	SV-104IS	80816	19 January 2025	113.5	113.5
NMD-B07	SVANTEK	SV-104IS	80817	19 January 2025	113.5	113.5
NMD-B08	SVANTEK	SV-104IS	80818	19 January 2025	113.5	113.5
NMD-B09	SVANTEK	SV-104IS	80829	19 January 2025	113.5	113.5
Acoustic Certified Value : Thailand Institute of Scientific and Technological Research (TISTR)					113.50± 0.10 dB	

Calibrated by :

Adul Dangklom

(Mr. Adul Dangklom)

Approved by :

Peera Detudom

(Mr. Peera Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจตุจักร เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72 Fax : (662) 513-4221 E-mail : sales@spscon.com, www.spscon.com

Noise Dose R_213-1/25

Noise Dose Meter Calibration Report

Acoustic Calibrator Data

Brand	SVANTEK	Number	SV 01/60
Model	SV34	Serial No.	33137
Calibration Range	114 dB, 1000 Hz	Last Calibration	06 August 2024
		Due Date	06 August 2025

Calibration Data

Sound Level Meter Data				Calibration Data		
SLM No.	Brand	Model	Serial No.	Date	Actual Reading [dB]	
					Before Adjustment	After Adjustment
NMD-B06	SVANTEK	SV-104IS	80816	07 April 2025	113.5	113.5
NMD-B07	SVANTEK	SV-104IS	80817	07 April 2025	113.6	113.5
NMD-B11	SVANTEK	SV-104IS	80831	07 April 2025	113.6	113.5
NMD-B12	SVANTEK	SV-104IS	80832	07 April 2025	113.5	113.5
NMD-B13	SVANTEK	SV-104IS	80834	07 April 2025	113.5	113.5
NMD-B14	SVANTEK	SV-104IS	80875	07 April 2025	113.5	113.5
NMD-B15	SVANTEK	SV-104IS	80880	07 April 2025	113.6	113.5
NMD-B16	SVANTEK	SV-104IS	106120	07 April 2025	113.5	113.5
NMD-B17	SVANTEK	SV-104IS	106122	07 April 2025	113.5	113.5
Acoustic Certified Value : Thailand Institute of Scientific and Technological Research (TISTR)					113.50± 0.10 dB	

Calibrated by :

Adul Dangklom

(Mr. Adul Dangklom)

Approved by :

Peer Detudom

(Mr. Peera Detudom)

ลำดับที่ 5

คุณภาพน้ำจากระบบบำบัดน้ำเสีย



IRPC PUBLIC COMPANY LIMITED

METROLOGY CENTER

299 Moo 5, Sukhumvit Road, Amphor Muang, Rayong, 21000 THAILAND
Tel. 0-3861-1333, 0-3861-3571-80 Ext. 4441, 4444 Fax. 0-3861-2812-3, 0-3889-8830



Certificate of Calibration

Reference : 30241275

Certificate No. : CL1-M255006

Issued by : Mass Laboratory

Page : 1 of 4

Object.	:	Electronic Balance
Manufacturer.	:	Sartorius
Ident. No.	:	EN-01-006
Model / Type.	:	TE214S / Single range
Serial No.	:	SWB25909250
Customer.	:	ALEX/ALPO (Env.) IRPC Public Company Limited. 299 Moo 5, Sukhumvit Road, Tumbon Chenong Nern, Amphor Muang, Rayong, 21000.
Date of Received.	:	24 January 2025
Date of Calibration.	:	24 January 2025
Place of Calibration	:	2nd Floor, Ethelene Building.

The reported uncertainty is based on a standard uncertainty multiplied by a coverage factor (k), providing a level of confidence of approximately 95%

Issued Date.

Approved by.

Calibrated by.

24 January 2025

(Taweesak Promsorn)

Head of the calibration laboratory

(Chakrit Cheepnurat)

Continuation of Calibration Certificate No. : CL1-M255006

Page : 2 of 4

Object	:	Electronic Balance
Manufacturer	:	Sartorius
Identification No.	:	EN-01-006
Model / Type	:	TE214S / Single range
Serial No.	:	SWB25909250
Calibration Range	:	0 g to 200 g
Accuracy	:	N/A
Division / Resolution	:	0.0001 g
Condition of Object	:	In Condition

ENVIRONMENT CONDITIONS :

Air Temperature	:	24.1 °C ± 0.1 °C
Relative Humidity	:	52.5 % ± 0.6 %
Atmospheric Pressure	:	1008.3 mbar ± 0.1 mbar

MEASUREMENT METHOD :

- The balance is calibrated using the procedure according to the instruction manual number S10325200-2212. calibration method is based on UKAS Lab 14.
- For multi-interval or multiple range instruments where intervals or ranges are switched automatically these measurements may only be required on one such interval / range.
- Balance calibration is performed by comparing the conventional mass values of the reference weights with the readings on the balance display.

TRACEABILITY :

Instrument	Model	Serial No.	Certificate No.	Due date
1. Standard weight Set 1 mg to 1 kg	Class F1	15891	CL1-M232036	15-May-25

Note : This reference standard is traceable to the International System of Units (SI) through the IRPC Metrology Center.

UNCERTAINTY OF MEASUREMENTS :

The uncertainty stated is the expanded uncertainty which results from multiplying the standard uncertainty by the coverage factor (k). It has been determined according to "M3003 the Expression of Uncertainty and Confidence in Measurement" This mean the value of the measured lies within the assigned range of values with a probability of approximately 95%.



MEASUREMENT RESULTS :

Balance Serial No. : SWB25909250

Range Capacity : 0 g to 210 g

Resolution : 0.0001 g

A 'Zero-Tracking' facility of Weighing machines.


☐ Enable. ☐ Disabled. ☒ N/A. (No Application)☐ Without adjustment.☐ Adjustment by internal calibration of Balance.☒ Adjustment using external weight. 200 g**1. Repeatability.**

Test Weight : 200 g

Measurement	Displayed value (g)
1	199.9999
2	199.9999
3	199.9999
4	200.0002
5	200.0002
6	200.0002
7	200.0002
8	200.0002
9	200.0002
10	200.0002
Average	200.0001
SD	0.00014

2. Eccentric or Off-centre loading.

Test Weight : 100 g

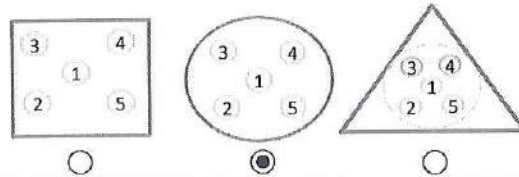

Load position	Displayed value (g)	Difference off-center (g)
1	100.0002	0.0000
2	100.0001	0.0001
3	100.0007	-0.0005
4	100.0006	-0.0004
5	100.0000	0.0002
Maximum difference off-Center		-0.0005

3. Effect of tare and/or balancing mechanism


Weight used for tare weight : 100 g

Nominal value (g)	Conventional mass (g)	Displayed value. (g)	Correction value. (g)
20	19.999920	20.0000	-0.0001
40	39.999850	39.9998	0.0000
60	59.999940	60.0001	-0.0002
80	79.999860	79.9999	0.0000
100	100.000110	100.0002	-0.0001

MEASUREMENT RESULTS :**4. Error of indication from nominal or conventional mass value.**

Nominal value (g)	Conventional Mass (g)	Displayed value (g)	Correction value (g)	Uncertainty \pm (g)	Coverage factor (k)
0.05	0.050006	0.0499	0.0001	0.00021	2.21
0.1	0.099999	0.1000	0.0000	0.00021	2.20
0.2	0.200004	0.2000	0.0000	0.00021	2.20
0.5	0.499995	0.5000	0.0000	0.00021	2.20
1	1.000027	1.0000	0.0000	0.00021	2.20
2	2.000041	2.0000	0.0000	0.00021	2.18
5	4.999956	4.9999	0.0001	0.00021	2.17
10	9.999880	10.0000	-0.0001	0.00022	2.13
20	19.999920	19.9999	0.0000	0.00023	2.11
50	50.000060	50.0001	0.0000	0.00040	2.01
100	100.000110	100.0005	-0.0004	0.00062	2.00
110	109.999990	110.0002	-0.0002	0.00064	2.00
120	120.000030	120.0002	-0.0002	0.00065	2.00
150	150.000170	150.0003	-0.0001	0.00074	2.00
200	199.999820	200.0000	-0.0001	0.00055	2.00

The graphs of correction values and uncertainties are shown as follows.

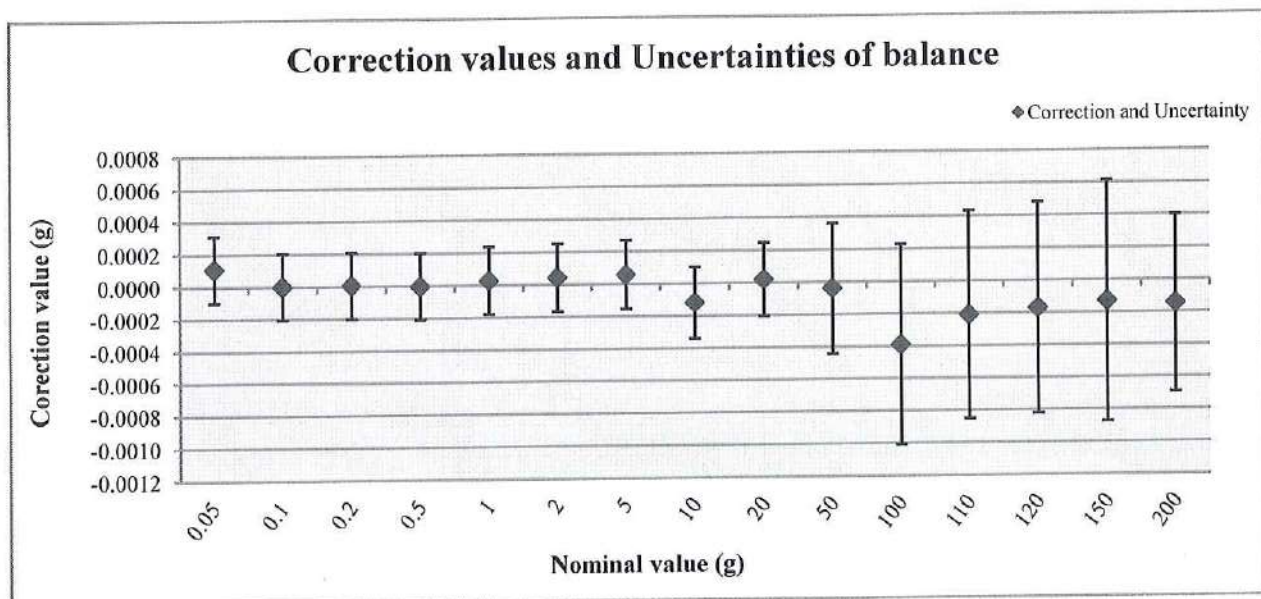

Remark : This result of calibration was found accurate as shown on date, place and for the unit under calibration only.

*** End of report ***

nd.



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3 : EQUIPMENT CALIBRATION AND TESTING SERVICES


534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250

TEL. 0-2717-3000 FAX. 0-2719-9484

Certificate of Testing

Cert.No.: 25TW84

Page.: 1 of 2

Equipment :	DO Meter
Manufacturer :	WTW
Model :	Oxi7310
Serial No. :	18020813
ID No. :	-
Received Date :	28 April 2025
Test Date :	29 April 2025
Reference :	2504-0708DC-10
Submitted by :	IRPC Public Company Limited 299 Moo.5, Sukhumvit Road, T.Cherngner, A.Muang, Rayong 21000
Laboratory Condition :	Temperature (25 ± 5) °C Humidity (50 ± 20) %
Test Procedure :	In - house method : CP-CH9 by Comparison Technique with Azide Modification Method
Tested by :	Walalak Sirithean 
Approved by :	<hr/> Approved Signatory
() Chakrit Waewwanjua () Ponpan Paipim (✓) Saithip Meangmai	
Issue Date :	30 April 2025



Cert.No.: 25TW84

Page.: 2 of 2

Condition of this result of calibration

1. Reference Standard Instruments :

This certification is traceable to the International System of Unit through the reference standards laboratory of Industrial Calibration Center, Technology Promotion Association (Thailand-Japan).

<u>Instruments</u>	<u>Serial No.</u>	<u>ID No.</u>	<u>Certificate No.</u>	<u>Due Date</u>
1. Burette	-	130BU10	25CG1126	18 Mar 2027
2. Balance	14233821	110RC001	24MM131	04 July 2025

2. Standard Material :-

<u>Material</u>	<u>Manufacturer</u>	<u>Lot.No.</u>	<u>Assay</u>
Sodium Thiosulfate 5-Hydrate AR	KEMAUS	2203162447	99.6%

Result : Dissolved Oxygen Meter Adjustment With Air 100 %

Dissolved Oxygen Probe No.: 24210014

Titration Method (Azide Modification Method) (mg/L)	DO Meter Reading (mg/L)	Standard Deviation (mg/L)
8.20	8.29	0.0055

This report was certified only for the instrument we tested. It is allowable to use for study
Intend to use for advertising and referral purpose is prohibited. This report may not be reproduced
other in full, without written approval of the laboratory

-o0o-

Calibration Certificate

Equipment:	COD Reactor	Job No.:	KSMT2501466
Model:	Digital PREP Cube	Received Date:	18 April 2025
Serial No.(or ID):	CBB0412050122 (EN-05-001)	Issued Date:	23 April 2025
Manufacturer:	SCP SCIENCE	Page:	1 of 4
Covers:	Open (Max)		
Holes:	25		

Customer

IRPC PUBLIC CO., LTD.
299 Moo 5, Sukhumvit Road, Tambol Choengneon, Amphur Muang, Rayong 21000 Thailand

Calibration Place

IRPC PUBLIC CO., LTD. (Gc Lab)
299 Moo 5, Sukhumvit Road, Tambol Choengneon, Amphur Muang, Rayong 21000 Thailand

Calibration Date

18 April 2025

Environment Condition

Temperature: 24 °C ± 0.2 °C
Humidity: 65 %RH ± 1.2 %RH

The Method used

In-house method, based on Direct Measurement with
Standard Thermometer



Traceability

This certificate is traceable to the SI Units maintained by
National Institute of Metrology (NIMT), Thailand through
SCIMET Co.,Ltd. Certificate No. C23250017

This certificate is issued the units of measurement according to the International System of Units (SI). It provides traceability of measurement to international or national standard or other recognized national standard laboratories.

The measurement uncertainty stated is the expanded uncertainty which is obtained from the standard uncertainty multiplied by the coverage factor ($k=2$) to provide a level of confidence of approximately 95%. It is determined in accordance with the Guide to Expression of Uncertainty in Measurement (GUM).


These results may be affected by deviations from specified conditions. The results relate only to the items tested, calibrated or sampled. The report shall not be reproduced except in full without approval of SCIMET Co., Ltd.


(Mr. Chattaphon Foithong)
Person in charge
(Mr. Thalerngkeat Pongngam)
Authorized signatory


Condition of reference standards instruments:

<u>Instruments</u>	<u>Model</u>	<u>S/N or ID.</u>	<u>Certificate No.</u>	<u>Due Date</u>
Datalogger 3	34970A	MY44075238	C23250017	28-Jan-2026

Condition of Calibration item : In Condition

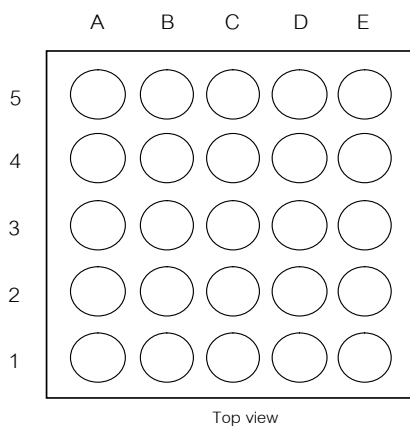

Location of standard



Sample test

Standard Installation Locations

The standard thermometer touches the lower end of the boring

Definitions

<i>Indicating Temperature:</i>	The average reading of indicating device which forms the integral part of the unit under calibration.
<i>Measured Temperature:</i>	The average reading of standards at any positions or location.
<i>Measured Stability:</i>	The one-half of greatest maximum difference of measured temperatures at any one probe.

Calibration Results:

Without Adjustment

Measured temperature at the spread locations:

Locations heating Block:	Setting (°C)	Unit Under Calibration (°C)
Single	152.0	152.0

Location heating Block:	Measured Temperature (°C)	Correction (°C)	Uncertainty (± °C)
A1	149.68	-0.32	0.30
A2	150.42	0.42	0.30
A3	151.10	1.10	0.28
A4	150.10	0.10	0.32
A5	149.68	-0.32	0.30
B1	150.41	0.41	0.32
B2	151.43	1.43	0.31
B3	151.25	1.25	0.29
B4	150.25	0.25	0.34
B5	151.10	1.10	0.29
C1	150.41	0.41	0.33
C2	151.13	1.13	0.29
C3	149.70	-0.30	0.31
C4	150.32	0.32	0.30
C5	149.95	-0.05	0.29
D1	149.48	-0.52	0.28
D2	150.14	0.14	0.29
D3	149.96	-0.04	0.29
D4	149.48	-0.52	0.28
D5	150.64	0.64	0.28
E1	148.86	-1.14	0.28
E2	148.98	-1.02	0.28
E3	149.53	-0.47	0.28
E4	148.94	-1.06	0.28
E5	148.87	-1.13	0.30

Characterization of the unit under calibration:

Locations heating Block	Desired	Unit Under Calibration (°C)		Measured Temperature (°C)
	(°C)	Setting	Reading	Stability (±°C)
Single	150.0	152.0	152.0	0.18

The End of Certificate

ใบตรวจสอบสภาพเครื่องควบคุมอุณหภูมิ

เลขที่ใบงาน: KSMT2501466

ชนิดเครื่องมือ: COD Reactor

รุ่น: Digital PREP Cube

หมายเลขเครื่อง: CBB0412050122 (EN-05-001)

ตรวจสอบ (รับ)		รายการตรวจเช็ค	ตรวจสอบ (ส่ง)		หมายเหตุ
18 Apr 2025			18 Apr 2025		
ปกติ	ไม่ปกติ		ปกติ	ไม่ปกติ	
		General			
<input checked="" type="checkbox"/>	<input type="checkbox"/>	1. สายไฟ	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	2. การทำงาน Main Switch	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	3. การทำงาน Selector Key	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	4. การแสดงผล Display	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	5. สภาพ Hole	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input type="checkbox"/>	<input type="checkbox"/>	6. สภาพฝาปิด	<input type="checkbox"/>	<input type="checkbox"/>	ไม่มี
<input checked="" type="checkbox"/>	<input type="checkbox"/>	7. สภาพตัวเครื่อง	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	8. สภาพแวดล้อม ณ สถานที่ตั้งเครื่อง	<input checked="" type="checkbox"/>	<input type="checkbox"/>	

ข้อแนะนำ :

Mr. Chattuphon Foithong

Service Engineer

Certificate No. C17240284

Calibration Certificate

Equipment:	Hot Air Oven	Job No.:	KSMT2402337
Model:	UF 55	Received Date:	04 September 2024
Serial No.(or ID):	B216.2858 (EN-05-033)	Issued Date:	10 September 2024
Manufacturer:	Memmert	Page:	1 of 3
Condition:	In Condition		
Ventilation Valve:	Closed	Shelves(pc.):	3

Customer

IRPC PUBLIC CO., LTD.
299 Moo 5, Sukhumvit Road, Tambol Choengneon, Amphur Muang, Rayong 21000 Thailand

Calibration Place

IRPC PUBLIC CO., LTD. (Envi Lab, instrument Room)
299 Moo 5, Sukhumvit Road, Tambol Choengneon, Amphur Muang, Rayong 21000 Thailand

Calibration Date

04 September 2024

Environment Condition

Temperature: 23.7 °C ± 1.0 °C
Humidity: 65.9 %RH ± 3.6 %RH

The Method used

In-house method, WI17, based on TLAS-G20

Traceability

This certificate is traceable to the SI Units maintained by
National Institute of Metrology (NIMT), Thailand through
SCIMET Co.,Ltd.Certificate No. C23240083

This certificate is issued the units of measurement according to the International System of Units (SI). It provides traceability of measurement to international or national standard or other recognized national standard laboratories.

The measurement uncertainty stated is the expanded uncertainty which is obtained from the standard uncertainty multiplied by the coverage factor ($k=2$) to provide a level of confidence of approximately 95%. It is determined in accordance with the Guide to Expression of Uncertainty in Measurement (GUM).

These results may be affected by deviations from specified conditions. The results relate only to the items tested, calibrated or sampled. The report shall not be reproduced except in full without approval of SCIMET Co., Ltd.




(Mr. Chanachol Moohammudrosol)

Person in charge



(Mr. Thalerngkeat Pongngam)

Authorized signatory

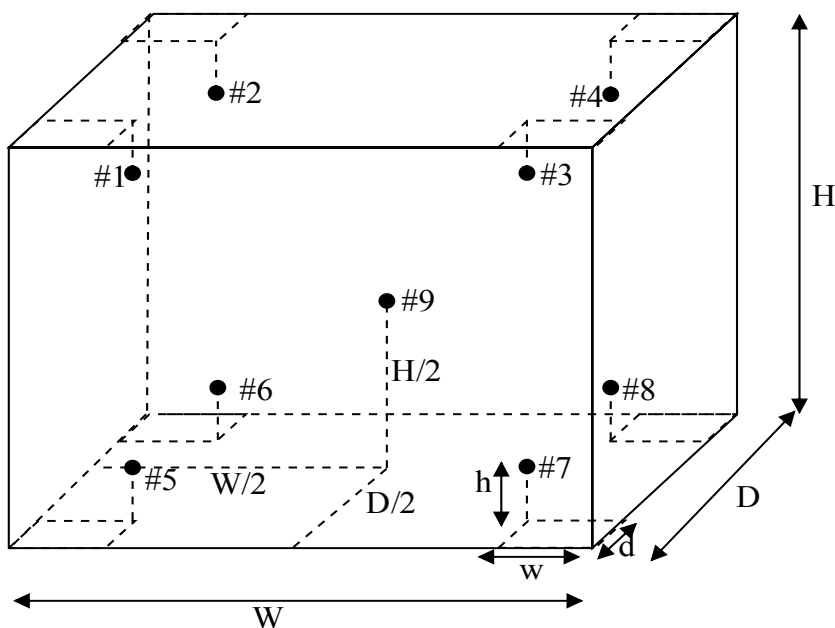

Standard Installation Locations

Volume (Calibration Zone)= 21 (Liters)

Inside chamber: $W = 40$ (cm) $D = 33$ (cm) $H = 40$ (cm)

Standard Locations (#1, #2, #3, #4): $w = 5$ (cm) $d = 5$ (cm) $h = 5$ (cm)

Standard Locations (#5, #6, #7, #8): $w = 5$ (cm) $d = 5$ (cm) $h = 5$ (cm)

#9: Geometric center of the chamber

Position of Std	#1	#2	#3	#4	#5	#6	#7	#8	#9
Channel of Logger	201	202	203	204	205	206	207	208	209

Definitions

Indicating Temperature: The average reading of indicating device which forms the integral part of the enclosure.

Measured Temperature: The average reading of standards at any positions or location.

Measured Uniformity: The maximum difference of measured temperatures between of any probes and the measured temperature at the reference location which are observed at same time or at close observation time as possible to determine the temperature pattern or homogeneity with the chamber at steady-state. The reference probe is preferably located in the geometric center of the chamber.

Measured Stability: The one-half of greatest maximum difference of measured temperatures at any one probe.

Overall Variation: The difference of maximum and minimum measured temperatures throughout observation time.

Calibration Results:

Without adjustment

Measurement Temperature at Spread Locations, Indicating of Unit Under Calibration: 104.0 °C

Locations	Measured Temperature (°C)	Correction (°C)	Uncertainty (± °C)
#1	104.09	0.09	0.39
#2	104.14	0.14	0.39
#3	104.40	0.40	0.39
#4	104.14	0.14	0.39
#5	103.55	-0.45	0.39
#6	104.16	0.16	0.39
#7	103.58	-0.42	0.39
#8	103.86	-0.14	0.39
#9	103.44	-0.56	0.39

Temperature Distribution

Desired (°C)	Setting (°C)	Indicating (°C)	Measured Temperature at Spread Locations (°C)									Uncertainty (± °C)*
			#1	#2	#3	#4	#5	#6	#7	#8	#9	
104.0	104.0	104.0	104.09	104.14	104.40	104.14	103.55	104.16	103.58	103.86	103.44	0.39

Chamber Characterization

Indicating (°C)	Measured Uniformity (°C)	Measured Stability (± °C)	Overall Variation (°C)
104.0	0.99	0.07	1.04

Note: * Maximum uncertainty of the each position

The End of Certificate

Statements of conformity:

This conformity certificate documents the validity of the following statements of conformity based on the measurement results of corresponding calibration certificate:

The correction of indication determined during calibration are under given measurement and environmental conditions and considering the expanded measurement uncertainty (coverage probability 95%) within the specification. The given measurement uncertainty already includes other all effects by according to the standard method, TLAS-G20. Therefore, those parameters have not

Tolerance and Decision rules:

Assessment of the conformity of the measurement device are done based on direct comparison of the relevant measurement results with the tolerances and decision rule are prescribed by the customer.

- Decision rule :** ☐ Choice A Binary Statement for Simple Acceptance Rule ($w = 0$), Specific Risk $< 50\%$ PFA.
- ☒ Choice B Non-binary statement with guard band ($w = 1 U$), Pass or Fail Specific Risk $< 2.5\%$ PFA and Condition Pass or Condition Fail Specific Risk $< 50\%$ PFA.
- ☐ Choice C Customer defined, Customers may define arbitrary multiple of r to have applied as guard band ($w = r U$) .
- ; PFA: Probability of False Accept




(Mr. Thalerngkeat Pongngam)

Authorized signatory

Without adjustment

Desired Temperature : 104.0°C

Tolerances : 1.0 °C

Measurement Temperature at Spread Locations, Indicating of Unit Under Calibration: 104.0 °C

Locations	Measured (°C)	Correction of UUC. (°C)	Guard band (W) (± °C)	Tolerance (± °C)	Conformity
#1	104.09	0.09	0.39	1.0	Pass
#2	104.14	0.14	0.39	1.0	Pass
#3	104.40	0.40	0.39	1.0	Pass
#4	104.14	0.14	0.39	1.0	Pass
#5	103.55	-0.45	0.39	1.0	Pass
#6	104.16	0.16	0.39	1.0	Pass
#7	103.58	-0.42	0.39	1.0	Pass
#8	103.86	-0.14	0.39	1.0	Pass
#9	103.44	-0.56	0.39	1.0	Pass

Correction of UUC.* = Measured Temperature - Desired Temperature

The validity of the statements of conformity cannot be guaranteed for different places of use, environmental conditions or improper use.


The End of Statements of Conformity

Corr_Distribution & Max_Measurement Uncertainty

Job_No. KSMT2402337

Without adjustment


Correction (°C)

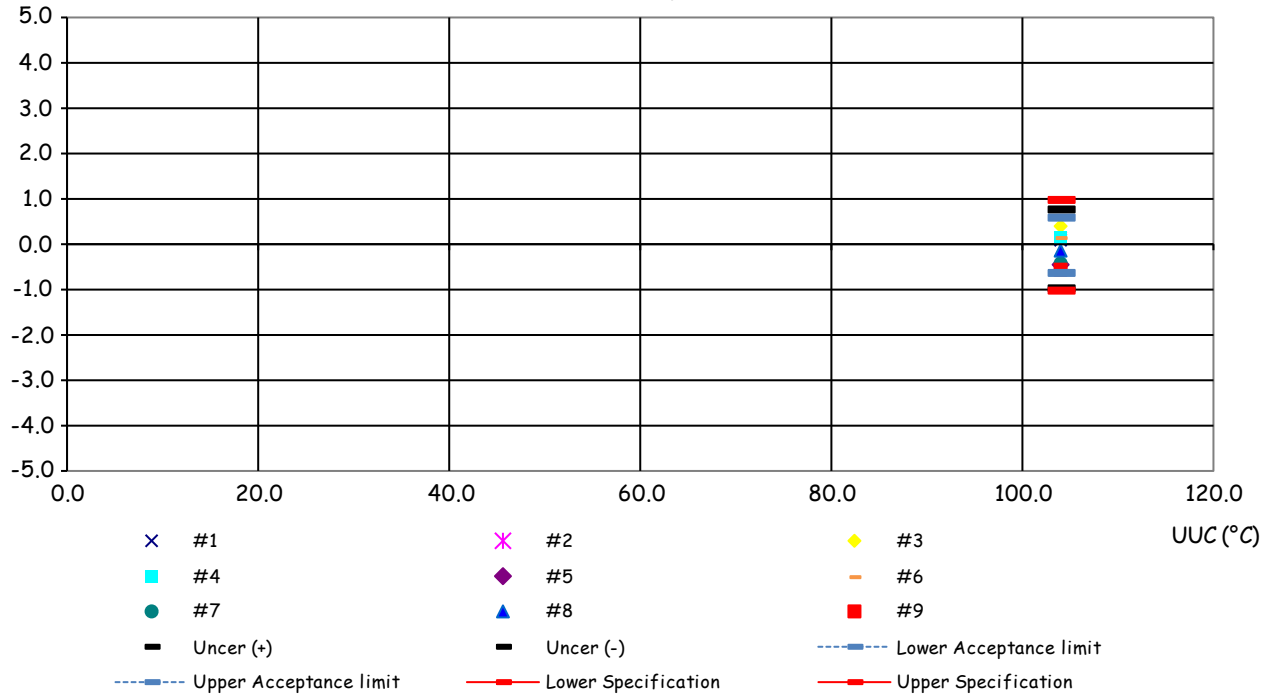


Temperature Distribution @ 104.0°C

Job_No. KSMT2402337

Without adjustment

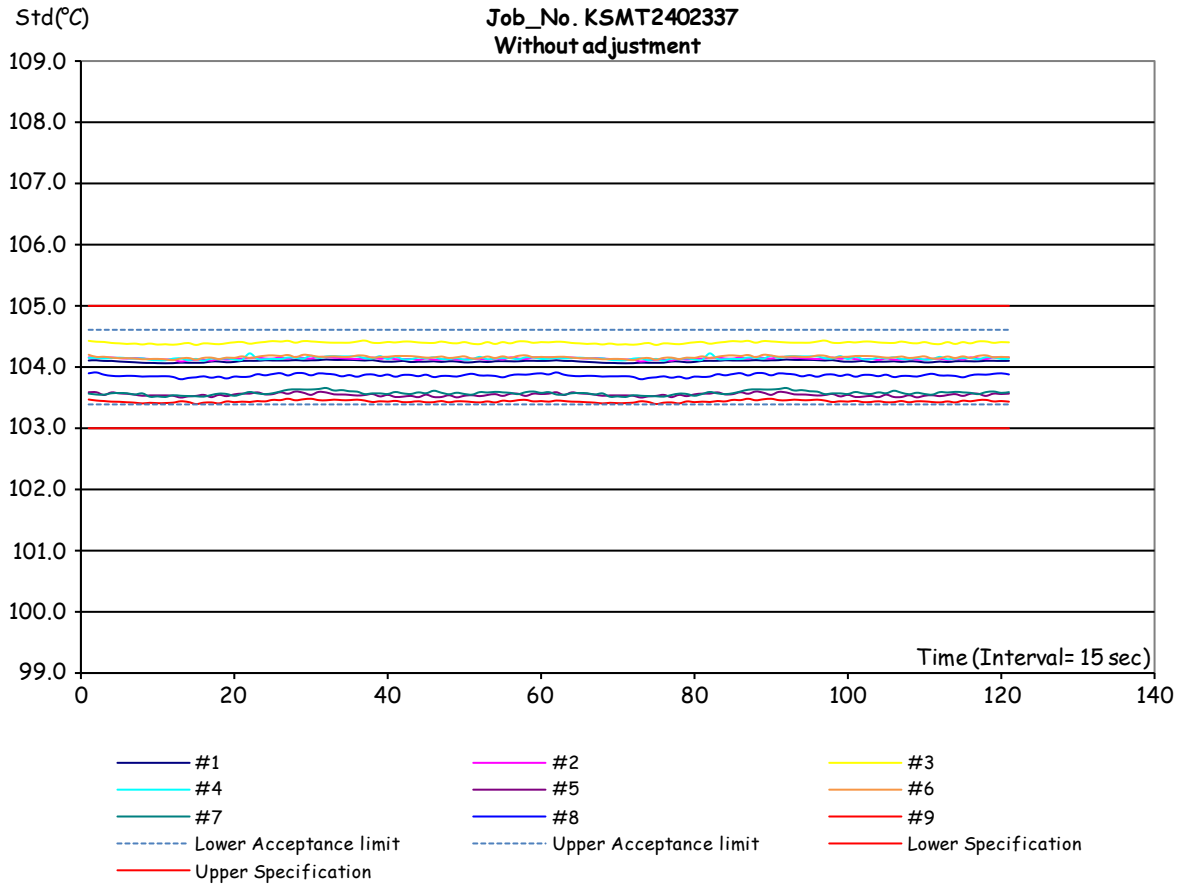



ใบตรวจสอบสภาพเครื่องควบคุมอุณหภูมิ

เลขที่ใบงาน: KSMT2402337

ชนิดเครื่องมือ: Hot Air Oven

รุ่น: UF 55

หมายเลขเครื่อง: B216.2858 (EN-05-033)

ตรวจสอบ (รับ)		รายการตรวจเช็ค	ตรวจสอบ (ส่ง)		หมายเหตุ
04 Sep 2024			04 Sep 2024		
ปกติ	ไม่ปกติ		ปกติ	ไม่ปกติ	
		General			
<input checked="" type="checkbox"/>	<input type="checkbox"/>	1. สายไฟ	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	2. การทำงาน Main Switch	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	3. การทำงาน Selector Key	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	4. การแสดงผล Display	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	5. การทำงาน พัดลม	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	6. สภาพ Lever of Ventilation valve	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	7. สภาพ Lever door open / close	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	8. สภาพ Door seal	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	9. การทำงานของระบบ Safety	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input type="checkbox"/>	<input type="checkbox"/>	10. การทำงานของระบบทำความเย็น	<input type="checkbox"/>	<input type="checkbox"/>	-
<input type="checkbox"/>	<input type="checkbox"/>	11. การทำงานของระบบทำความร้อน	<input type="checkbox"/>	<input type="checkbox"/>	-
<input checked="" type="checkbox"/>	<input type="checkbox"/>	12. สภาพตัวเครื่อง	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	13. สภาพแวดล้อม ณ สถานที่ตั้งเครื่อง	<input checked="" type="checkbox"/>	<input type="checkbox"/>	

ข้อแนะนำ :

Mr. Chanachol Moohammudrosol

Service Engineer

Certificate No. C08250095

Calibration Certificate

Equipment:	pH METER	Job No.:	KSMT2501889
Model:	HQ40d	Received Date:	27 May 2025
Serial No.(or ID):	130500088588 (L09-AT-SP003-A2)	Issued Date:	27 May 2025
Manufacturer:	Hach	Page:	1 of 3
Condition:	In Condition		

Customer

IRPC PUBLIC CO., LTD.
299 Moo 5, Sukhumvit Road, Tambol Choengneon, Amphur Muang, Rayong 21000 Thailand

Calibration Place

IRPC PUBLIC CO., LTD. (Gc Lab)
299 Moo 5, Sukhumvit Road, Tambol Choengneon, Amphur Muang, Rayong 21000 Thailand

Calibration Date

27 May 2025

Environment Condition

Temperature: 25.2 °C ± 0.2 °C
Humidity: 66.2 %RH ± 1.7 %RH

The Method used

In-house method, WI08, based on ASTM E 70-07


Traceability

This certificate is traceable to SI Units, Sample Test is assured through primary measurement method Harned cell, through CPAchem Ltd. (ISO17034) Certificate No. 1066714, 1066715, 1066716, pH Scale and Temperature test are traceable to the SI Units maintained by National Institute of Metrology (NIMT), Thailand through Industrial Foundation Electrical and Electronics Institute Certificate No. CA20250010EA, through SCIMET Co., Ltd. Certificate No.C23240075

This certificate is issued the units of measurement according to the International System of Units (SI). It provides traceability of measurement to international or national standard or other recognized national standard laboratories.


The measurement uncertainty stated is the expanded uncertainty which is obtained from the standard uncertainty multiplied by the coverage factor ($k=2$) to provide a level of confidence of approximately 95%. It is determined in accordance with the Guide to Expression of Uncertainty in Measurement (GUM).

These results may be affected by deviations from specified conditions. The results relate only to the items tested, calibrated or sampled. The report shall not be reproduced except in full without approval of SCIMET Co., Ltd.



(Mr. Chattuphon Foithong)

Person in charge



(Mr. Thalerngkeat Pongngam)

Authorized signatory

Condition of reference standards Instruments / CRM:

<u>Instruments</u>		<u>Model or S/N.</u>	<u>Certificate No.</u>	<u>Due date</u>
Standard Buffer solution	4.007 pH	PH216.L5	1066714	18-Jan-27
Standard Buffer solution	6.965 pH	PH107.L5	1066715	18-Jan-26
Standard Buffer solution	10.010 pH	PH220.L5	1066716	18-Jan-26
DC Voltage and Current Calibrator / XITRON		2000MN	CA20250010EA	19-Jan-26
Digital Thermometer		376	C23240075	30-Jul-25

Calibration Results:

pH Scale

Input (mV)	pH Meter Reading			Uncertainty of Measurement (mV)	Coverage Factor (<i>k</i>)
	(mV)	Error (mV)	(pH)		
414.12	414.0	-0.12	0.010	0.065	2.00
354.96	354.9	-0.06	1.010	0.065	2.00
295.80	295.8	0.00	2.008	0.065	2.00
236.64	236.5	-0.14	3.006	0.065	2.00
177.48	177.6	0.12	4.005	0.065	2.00
118.32	118.3	-0.02	5.003	0.065	2.00
59.16	59.1	-0.06	6.002	0.065	2.00
0.00	0.0	0.00	7.000	0.065	2.00
-59.16	-59.2	-0.04	7.999	0.065	2.00
-118.32	-118.3	0.02	8.997	0.065	2.00
-177.48	-177.5	-0.02	9.995	0.065	2.00
-236.64	-236.6	0.04	10.994	0.065	2.00
-295.80	-295.8	0.00	11.992	0.065	2.00
-354.96	-354.9	0.06	12.990	0.065	2.00
-414.12	-414.1	0.02	13.990	0.065	2.00

Electrode Test Results*

The three-point calibration using three standard buffer solutions; pH 4.007 , pH 6.965 and pH 10.010

The practical slope of the pH electrode; 58.37 (mV/pH), 98.66%

The zero point of the pH electrode; 6.91 (pH)

Sample Test Results

Electrode Serial No.: 241662611624

Model: PHC201

Manufacturer: Hach

Standard Buffer Solution (pH)	Unit Under Calibration (pH)	Difference (pH)	Uncertainty of Measurement (pH)	Coverage Factor (<i>k</i>)
4.007	3.993	-0.014	0.0068	2.18
6.965	6.990	0.025	0.0090	2.00
10.010	9.998	-0.012	0.0077	2.00

Temperature Electrode

Dimension of Probe;

Length : 120 mm
Diameter : 12 mm
Immersion Depth : 80 mm

STD. Reading (°C)	UUC. Reading (°C)	Correction of UUC (°C)	Uncertainty of Measurement (±°C)	Coverage Factor (<i>k</i>)
24.96	25.1	-0.14	0.21	2.00

* Calibration Marked for Electrode Test" Not TISI Accredited " in this Certificate have been included for completeness.

The End of Certificate

Statements of conformity:

This conformity certificate documents the validity of the following statements of conformity based on the measurement results of corresponding calibration certificate:

The error of temperature determined during calibration are under given measurement and environmental conditions and considering the expanded measurement uncertainty (coverage probability 95%) within the specification. The given measurement uncertainty already includes other all effects by according to the standard method, ASTM E 70-07. Therefore, those parameters have not been assessed separately.

Tolerance and Decision rules:

Assessment of the conformity of the measurement device are done based on direct comparison of the relevant measurement results with the tolerances and decision rule are prescribed by the customer.

- Decision rule :** ☐ Choice A Binary Statement for Simple Acceptance Rule ($w = 0$), Specific Risk $< 50\%$ PFA
☒ Choice B Non-binary statement with guard band ($w = 1 U$), Specific Risk $< 2.5\%$ PFA
☐ Choice C Customer defined, Customers may define arbitrary multiple of r to have applied as guard band ($w = r U$) .
; PFA – Probability of False Accept



(Mr. Thalerngkeat POUNGNGAM)

Authorized signatory

pH Scale

Tolerance : 1 mV

Input (mV)	pH Meter Reading			Guard Band (w) (mV)	Tolerance (mV)	Conformity
	(mV)	Error (mV)	(pH)			
414.12	414.0	-0.12	0.010	0.065	1.0	Pass
354.96	354.9	-0.06	1.010	0.065	1.0	Pass
295.80	295.8	0.00	2.008	0.065	1.0	Pass
236.64	236.5	-0.14	3.006	0.065	1.0	Pass
177.48	177.6	0.12	4.005	0.065	1.0	Pass
118.32	118.3	-0.02	5.003	0.065	1.0	Pass
59.16	59.1	-0.06	6.002	0.065	1.0	Pass
0.00	0.0	0.00	7.000	0.065	1.0	Pass
-59.16	-59.2	-0.04	7.999	0.065	1.0	Pass
-118.32	-118.3	0.02	8.997	0.065	1.0	Pass
-177.48	-177.5	-0.02	9.995	0.065	1.0	Pass
-236.64	-236.6	0.04	10.994	0.065	1.0	Pass
-295.80	-295.8	0.00	11.992	0.065	1.0	Pass
-354.96	-354.9	0.06	12.990	0.065	1.0	Pass
-414.12	-414.1	0.02	13.990	0.065	1.0	Pass

Sample Test

Tolerance : 0.05 pH

The three-point calibration using three standard buffer solutions; pH 4.007 , pH 6.965 and pH 10.010

Standard Buffer Solution (pH)	Unit Under Calibration (pH)	Difference (pH)	Guard band (w) (pH)	Tolerance (pH)	Conformity
4.007	3.993	-0.014	0.0068	0.050	Pass
6.965	6.990	0.025	0.0090	0.050	Pass
10.01	9.998	-0.012	0.0077	0.050	Pass

The validity of the statements of conformity cannot be guaranteed for different places of use, environmental conditions or improper use.

The End of Statements of Conformity

ใบตรวจสอบสภาพเครื่อง pH Meter

เลขที่ใบงาน: KSMT2501889

ชนิดเครื่องมือ: pH METER

รุ่น: HQ40d

หมายเลขเครื่อง: 130500088588

ตรวจสอบ (รับ)		รายการตรวจเช็ค	ตรวจสอบ (ส่ง)		หมายเหตุ
27 May 2025			27 May 2025		
ปกติ	ไม่ปกติ		ปกติ	ไม่ปกติ	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	1. ความสมบูรณ์เครื่อง	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	2. ความสะอาด (ช่องใส่ตัวอย่าง, ภายใน-นอกเครื่อง)	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	3. สวิตช์ ปิด – เปิด เครื่อง (On-Off Swicth)	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	4. ปุ่มกด (Keypad)	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	5. หน้าจอ (Display, Screen Contrast)	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	6. อิเล็กโทรด (Electrode and Connection Cable)	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	7. สายอิเล็กโทรด	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input type="checkbox"/>	<input type="checkbox"/>	8. ระดับสารละลายใน Electrode (Level KCl)	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	9. ฝาปิดกันปลาย Electrode (Dust Protection Hood)	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input type="checkbox"/>	<input type="checkbox"/>	10. ขาจับอิเล็กโทรด (Stand)	<input type="checkbox"/>	<input type="checkbox"/>	-

เพิ่มเติม/ข้อแนะนำ :

Mr. Chattuphon Foithong
Service Engineer