

## ภาคผนวกที่ 4

---

### เอกสารการสอบเทียบความถูกต้องของเครื่องมือตรวจวัดคุณภาพสิ่งแวดล้อม

---

- ลำดับที่ 1    คุณภาพอากาศในบรรยากาศ
- ลำดับที่ 2    คุณภาพอากาศจากแหล่งกำเนิด
- ลำดับที่ 3    คุณภาพน้ำ
- ลำดับที่ 4    ระดับเสียงทั่วไป
- ลำดับที่ 5    ระดับเสียงในสถานประกอบการ

**ตารางสรุปรายการเอกสารการสอบเทียบความถูกต้องของเครื่องมือเก็บตัวอย่าง  
และเครื่องมือตรวจวิเคราะห์คุณภาพสิ่งแวดล้อม**

รายการตรวจวัด	เครื่องมือเก็บตัวอย่าง ชื่อเครื่องมือ	เครื่องมือตรวจวิเคราะห์ ชื่อเครื่องมือ
<b>1. คุณภาพอากาศในบรรยากาศ</b>		
TSP	High Volume Air Sampler Rec No. Blower No. R01, R11, R13	Digital Balance
PM <sub>10</sub>	High Volume Air Sampler Rec No. Blower No. R06, R07, R08	Digital Balance
SO <sub>2</sub>	Serial No. CM06280010, 1310957747, 1749, TRS1064, 76	Serial No. CM06280010, 1310957747, 1749, TRS1064, 76
NO <sub>x</sub>	Serial No. 1170530044, CM13090047, 2286, 4412, 1977	Serial No. 1170530044, CM13090047, 2286, 4412, 1977
<b>2. คุณภาพอากาศจากแหล่งกำเนิด</b>		
Total Suspended Particulate	Console No.R03, R05 Pitot Tube No. B08, B38, B45	Digital Balance
Oxides of Nitrogen	Vacuum Gauge	Spectrophotometer
Sulfur Dioxide	Personal Pump SKC No.B71, B72, R13, R35 Rotameter No.H-R02, H-R03	-
Carbon Monoxide	Personal Pump SKC No.B72, B71, R37, R43 Rotameter No.H-R02, H-R03	CO Analyzer No.R02
Lead	Console No.R03, R05 Pitot Tube No.B08, B38, B45	ICP
Mercury	Console No.R03, R05 Pitot Tube No.B08, B38, B45	AAS
Hydrogen sulfide	Personal Pump SKC No.B68 Rotameter No.H-R02	-
<b>3. คุณภาพน้ำ</b>		
pH	-	pH Meter
TSS	-	Digital Balance
TDS	-	Digital Balance
BOD <sub>5</sub>	-	BOD Analyzer
COD	-	COD Reactor
Grease & Oil	-	Digital Balance
Hydrogen Sulfide	-	-
Antimony	-	ICP
Arsenic	-	AAS
Barium	-	ICP

**ตารางสรุปรายการเอกสารการสอบเทียบความถูกต้องของเครื่องมือเก็บตัวอย่าง  
และเครื่องมือตรวจวิเคราะห์คุณภาพสิ่งแวดล้อม (ต่อ)**

รายการตรวจวัด	เครื่องมือเก็บตัวอย่าง	เครื่องมือตรวจวิเคราะห์
	ชื่อเครื่องมือ	ชื่อเครื่องมือ
<b>3. คุณภาพน้ำ (ต่อ)</b>		
Beryllium	-	ICP
Cadmium	-	ICP
Total Chromium	-	ICP
Trivalent Chromium	-	Spectrophotometer
Hexavalent Chromium	-	Spectrophotometer
Lead	-	ICP
Manganese	-	ICP
Mercury	-	AAS
Nickel	-	ICP
Selenium	-	AAS
Silver	-	ICP
Vanadium	-	ICP
Zinc	-	ICP
Total Petroleum Hydrocarbon (C5-C35)		
- TPH (C5-C8)	-	GC/MS
- TPH (C>8-C16)	-	GC/MS
- TPH (C>16-C35)	-	GC/MS
<b>4. ระดับเสียงในบรรยากาศ</b>		
$L_{eq}$ 5 min, $L_{eq}$ 1 hr, $L_{eq}$ 24 hr,	Acoustic Calibrator	-
$L_{max}$ , $L_{90}$ และ $L_{dn}$	Sound Level Meter ACO-R30, R33, R35	-
<b>5. ระดับเสียงในสถานประกอบการ</b>		
$L_{eq}$ 8 hr และ $L_{max}$	Acoustic Calibrator	-
	Sound Level Meter ACO-B41, R52	-

ลำดับที่ 1

คุณภาพอากาศในบรรยากาศ



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด

S.P.S. CONSULTING SERVICE CO., LTD.

7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900

7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900

Tel : (662) 939-4370-72 Fax : (662) 513-4221 E-mail : sale@spscon.com, www.spscon.com

## High Volume Air Sampler Calibration Report

Calibration Method : Multipoint Orifice Flow Transfer Standard

Model : TE 5025A

S/N : 3611

### Calibration Data

High Volume Air Sampler Data		Calibration Data		
Recorder No.	Blower No.	Date	Actual Flowrate (ft <sup>3</sup> /min)	R <sup>2</sup>
B35	B35	05/02/2025	y = 1.163x-3.579	0.997
B36	B36	05/02/2025	y = 1.130x-2.116	0.999
B37	B37	04/02/2025	y = 1.146x-2.265	0.996
B38	B38	04/02/2025	y = 1.156x-6.034	0.998
B39	B39	03/02/2025	y = 1.151x-3.366	0.998
B40	B40	03/02/2025	y = 1.174x-4.582	0.999
B41	B41	06/02/2025	y = 1.123x-1.633	0.997
B42	B42	03/02/2025	y = 1.149x-3.382	0.997
B43	B43	03/02/2025	y = 1.137x-2.074	0.997
B44	B44	03/02/2025	y = 1.155x-1.460	0.999
R01	R01	04/02/2025	y = 1.121x-3.007	0.999
R02	R02	03/02/2025	y = 1.159x-5.099	0.999
R03	R03	05/02/2025	y = 1.138x-2.774	0.998
R04	R04	05/02/2025	y = 1.118x-2.575	0.999
R05	R05	03/02/2025	y = 1.136x-1.720	0.998
R06	R06	05/02/2025	y = 1.154x-2.706	0.997
R07	R07	03/02/2025	y = 1.037x+1.361	0.999
R08	R08	03/02/2025	y = 1.146x-3.762	0.996
R09	R09	05/02/2025	y = 1.121x-2.360	0.997
R10	R10	05/02/2025	y = 1.180x-4.626	0.999
R11	R11	05/02/2025	y = 1.147x-3.861	0.996
R12	R12	03/02/2025	y = 1.128x-4.676	0.998
R13	R13	04/02/2025	y = 1.135x-4.055	0.999
R14	R14	04/02/2025	y = 1.153x-3.122	0.997
R15	R15	03/02/2025	y = 1.161x-5.223	0.998
R16	R16	03/02/2025	y = 1.187x-6.674	0.999
R17	R17	03/02/2025	y = 1.120x-1.730	0.999
R18	R18	03/02/2025	y = 1.146x-2.347	0.998
R19	R19	06/02/2025	y = 1.161x-5.195	0.999
R20	R20	06/02/2025	y = 1.134x-3.449	0.998

Calibrated by :

Adul Dangklom  
(Mr. Adul Dangklom)

Approved by :

Peera Detudom  
(Mr. Peera Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด

S.P.S. CONSULTING SERVICE CO., LTD.

7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจตุจักร กรุงเทพฯ 10900

7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900

Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

## High Volume PM-10 Air Sampler Calibration Report

Calibration Method : Multipoint Orifice Flow Transfer Standard

Model : TE 5025A

S/N : 3611

### Calibration Data

High Volume PM-10 Data		Calibration Data		
Recorder No.	Blower No.	Date	Actual Flowrate (ft <sup>3</sup> /min)	R <sup>2</sup>
R01	R01	04/02/2025	$y = 1.168x - 5.536$	0.996
R02	R02	04/02/2025	$y = 1.116x - 2.200$	0.998
R03	R03	03/02/2025	$y = 1.160x - 5.911$	0.997
R04	R04	03/02/2025	$y = 1.129x - 4.829$	0.999
R05	R05	03/02/2025	$y = 1.119x - 3.825$	0.998
R06	R06	05/02/2025	$y = 1.125x - 1.580$	0.997
R07	R07	06/02/2025	$y = 1.152x - 2.503$	0.997
R08	R08	03/02/2025	$y = 1.114x - 1.275$	0.996
R09	R09	03/02/2025	$y = 1.130x - 4.187$	0.999
R10	R10	05/02/2025	$y = 1.151x - 2.832$	0.998
R11	R11	05/02/2025	$y = 1.134x - 2.692$	0.997
R12	R12	05/02/2025	$y = 1.158x - 4.761$	0.996
R13	R13	03/02/2025	$y = 1.137x - 3.435$	0.999
R14	R14	03/02/2025	$y = 1.126x - 2.499$	0.996
R15	R15	04/02/2025	$y = 1.111x - 3.285$	0.999
R16	R16	04/02/2025	$y = 1.124x - 0.808$	0.996
R17	R17	04/02/2025	$y = 1.141x - 3.412$	0.999
R18	R18	03/02/2025	$y = 1.115x - 3.615$	0.998
R19	R19	03/02/2025	$y = 1.117x - 0.234$	0.996
R20	R20	06/02/2025	$y = 1.146x - 4.675$	0.997

Calibrated by :

Adul Dangklom  
(Mr. Adul Dangklom)

Approved by :

Peera Detudom  
(Mr. Peera Detudom)





CERTIFICATE No : 25M2254

REFERENCE No : 76365-1

PAGE : 1 OF 2

## Certificate of Calibration

**EQUIPMENT** : DIGITAL BALANCE

**MANUFACTURER** : METTLER TOLEDO

**MODEL** : XS105DU

**SERIAL No** : 1126422905

**ID No** : BA05/50

**CONDITION AS RECEIVED** : USED ITEM

**SUBMITTED BY** : S.P.S. CONSULTING SERVICE CO., LTD.  
7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN RD.,  
JOMPOL, CHATUCHAK, BANGKOK 10900

**CALIBRATED BY** : ATSAWIN Y.

**CALIBRATION DATE** : 07-Mar-25

**APPROVED BY** :   
PONGSAK J.

**ISSUED DATE** : 13-Mar-25

**RECEIVED DATE** : 07-Mar-25

THIS CERTIFICATE MAY NOT BE REPRODUCED OTHER THAN IN FULL EXCEPT WITH THE PRIOR WRITTEN APPROVAL OF  
QUALITY CALIBRATION CO., LTD.







CERTIFICATE No : 25M2254

PAGE : 2 OF 2

## Calibration Report

EQUIPMENT : DIGITAL BALANCE MODEL : XS105DU  
MANUFACTURER : METTLER TOLEDO S/N : 1126422905  
ID No : BA05/50 RECEIVED DATE : 07-Mar-25  
AIR PRESSURE : 1009mbar  $\pm$  1mbar CALIBRATION DATE : 07-Mar-25  
AMBIENT TEMPERATURE : 24°C  $\pm$  1°C RELATIVE HUMIDITY : 54 %RH  $\pm$  10 % RH

### CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED BY ACCORDING TO UKAS LAB 14 EDITION 6:2019 BY USING KNOWN WEIGHT STANDARD WEIGHT. THE BALANCE WAS NOT ADJUSTED BEFORE CALIBRATION. THE BALANCE HAS NO ZERO TRACKING FUNCTION. REPEATABILITY WAS MEASURED BY USING 10 REPEATED MEASUREMENTS. LINEARITY WAS MEASURED COVERING 10 POINTS, EVENLY SPREAD OVER THE RANGE. THE INSTRUMENT WAS SET ZERO BEFORE PERFORMING THE LINEARITY TEST. OFF-CENTER LOADING WAS MEASURED BY USING STANDARD WEIGHTS PLACED ON THE PAN AND MOVED TO VARIOUS POSITIONS ON THE PAN.

### 2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) STANDARD WEIGHT SET	E2	QK-I-151	C02250116	28-Jan-27
2) STANDARD WEIGHT	E2	15843	C02250117	29-Jan-27

3. THE CERTIFICATE IS VALID FOR THE ITEM CALIBRATED AS SHOWN ON THE DATE AND PLACE OF CALIBRATION ONLY.

4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.

5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-

- NATIONAL INSTITUTE OF METROLOGY (THAILAND)

### RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

1. ZERO SETTING FUNCTION : NORMAL


2. TARE FUNCTION : NORMAL

3. REPEATABILITY OF READING AT 120 g WAS 0.000055 g

4. DEPARTURE FROM NOMINAL VALUE/ LINEARITY

NOMINAL VALUE (g)	BALANCE READING (g)	CORRECTION (g)	UNCERTAINTY ( $\pm$ g)
0.00	0.00000	0.00000	0.000065
0.02	0.01999	0.00001	0.000065
0.10	0.10001	-0.00001	0.000066
0.20	0.20001	-0.00001	0.000066
0.50	0.50002	-0.00002	0.000065
1.00	1.00003	-0.00003	0.000066
2.00	2.00001	-0.00001	0.000067
5.00	5.00002	-0.00002	0.000068
10.00	10.00000	0.00000	0.000070
20.00	20.00004	-0.00004	0.000078
50.00	50.00000	0.00000	0.00013
100.00	100.00001	-0.00001	0.00019
120.00	120.00002	-0.00002	0.00022

### 5. OFF CENTER LOADING ERROR



POINT	READING (g)
1	50.0000
2	50.0000
3	50.0000
4	50.0000
5	50.0000
OFF-CENTER LOADING	0.0000

NOTE: THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR  $k=2$ , PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT





Job Number :	J092500024	Customer Name :	IRPC
Equipment :	Micro Mobile AQMs	Contact Name :	Khun Wirasak Khumsuk
Model :	Micro Mobile AQMs	Telephone Number :	081-803-0475
Serial Number :	Micro Mobile3	E-mail address/Fax. :	<a href="mailto:wirasak.k@irpc.co.th">wirasak.k@irpc.co.th</a>
Working Date :	08 May 2025	Working Hour :	4 Hours

## Service Report

Working Scope:

รถเคลื่อนที่ AQMs micro#3 หยุดตรวจวัดอากาศ ปิดสถานี อยู่ที่ อนามัยหนองจอก จึงได้เข้าทำการตรวจเช็ค

Physical Checking:

- ตรวจเช็ค Data logger พบว่าทำงานได้ปกติ
- ตรวจเช็ค Diagnostic of all analyzers อยู่ในเกณฑ์ปกติ
- ตรวจเช็ค Reading of all analyzers และ Met sensor พบว่าปกติ
- ตรวจเช็ค เครื่องวัดฝุ่น PM-10 พบว่าทำงานได้ปกติ
- ตรวจเช็ค เครื่อง THC analyzer พบว่าทำงานได้ปกติ
- ตรวจเช็ค การทำงานของระบบไฟฟ้า และ UPS พบว่าทำงานได้ปกติ
- ทำความสะอาดภายในสถานี และ บริเวณรอบสถานี

Correction working:


Part Replacement:

- 
- 

Addition Recommended:

-- End --

Serviced by :	ชินโรส มุขโรจน์	Serviced Date :	08 May 2025
Approved by:		Approved Date :	08 May 2025



บริษัท คิว-ซี โซลูชั่นส์ จำกัด

7/409 ซอยวิภาวดีรังสิต 36 ถนนวิภาวดีรังสิต แขวงจตุจักร เขตจตุจักร กรุงเทพฯ 10900

โทรศัพท์ : (662) 939-5711 (12 Lines) โทรสาร : (662) 939-4207-8

Website <http://www.qshe.co.th> E-mail-address: [info@qshe.co.th](mailto:info@qshe.co.th)

## General Checking

Equipment : Micro Mobile AQMS

Model : -

Serial Number : -

Manufacturer : -

Item	Description	Set-Point Value	Status & Value	Remark
	<u>On Mobile</u>			
1	Air conditioner operation	OK	OK	
2	Mobile temperature	25-27 °C	25-27 °C	
3	Lighting system	OK	OK	
4	Lamp in sampling box	OK	OK	
5	Sampling probe	Clean	Clean	
6	Blower	OK	OK	
7	Drain liquid in tank	Drain	Drain	
8	Compressor tank set pressure	80 psi	80 psi	
9	Zero air compressor operation	OK	OK	
10	Silica gel for dry air of NO <sub>x</sub> analyzer	OK	OK	
11	UPS 6 KVA	Bypass	Bypass	
12	Data logger	OK	OK	
13	Ventilation fan	OK	OK	
14	Power cable	OK	OK	
15	Hydrogen Gas	>500 psi	2000/45 psi	
16	Standard gas#1 (NO,SO <sub>2</sub> ,HC,CO)	>500 psi	300/22 psi	

Note :



บริษัท คิว-ซี โซลูชั่นส์ จำกัด

7/409 ซอยวิภาวดีรังสิต 36 ถนนวิภาวดีรังสิต แขวงจตุจักร เขตจตุจักร กรุงเทพฯ 10900

โทรศัพท์ : (662) 939-5711 (12 Lines) โทรสาร : (662) 939-4207-8

Website <http://www.qshe.co.th> E-mail-address: [info@qshe.co.th](mailto:info@qshe.co.th)

NO-NO<sub>2</sub>-NO<sub>x</sub> AnalyzerEquipment : NO-NO<sub>2</sub>-NO<sub>x</sub> analyzer.

Model : 42i

Serial Number : CM13090047

Manufacturer : Thermo

## Diagnostic test value

Parameter	Observed value		Unit	Nominal range
	Before	After		
<b>Sample reading</b>				
NO reading			ppb	
NO <sub>x</sub> reading			ppb	
<b>Range</b>			ppb	50 to 1000 ppb
<b>Averaging Time</b>			Sec	10 to 300 Sec
<b>Calibration Factors</b>				
NO BKG. ppb			ppb	0 to 60
NO <sub>x</sub> BKG. ppb			ppb	0 to 60
NO COEF.			-	1.0 ± 0.3
NO <sub>x</sub> COEF.			-	1.0 ± 0.3
NO <sub>2</sub> COEF.			-	1.0 ± 0.3
<b>Instrument Controls</b>				
Ozonator				On/Off
PMT Supply				On/Off
Auto/Manual Mode				NO/NO <sub>x</sub> , NO, NO <sub>x</sub>
Baud Rate			bps	1200 to 9600
Temp Compensation			-	On/Off
Pressure Compensation			-	On/Off
Screen Contrast			%	0 to 100
Service Mode			-	On/Off, Up to used
<b>Diagnostics</b>				
<b>Voltages</b>				
<b>Motherboard voltages:</b>				
3.3 Supply			Vdc	3.3 ± 1 Vdc
5.0 Supply			Vdc	5.0 ± 1 Vdc
15.0 Supply			Vdc	15.0 ± 1 Vdc
24.0 Supply			Vdc	24.0 ± 1 Vdc
-3.3 Supply			Vdc	-3.3 ± 1 Vdc
<b>Interface board voltages:</b>				
PMT Supply			Vdc	-400 to -1200 Vdc
3.3 Supply			Vdc	3.3 ± 1 Vdc
5.0 Supply			Vdc	5.0 ± 1 Vdc
15.0 Supply			Vdc	15.0 ± 1 Vdc
P15.0 Supply			Vdc	15.0 ± 1 Vdc
24.0 Supply			Vdc	24.0 ± 1 Vdc
-15.0 Supply			Vdc	-15.0 ± 1 Vdc
<b>Temperatures</b>				
Internal			°C	15 °C to 45 °C
Chamber			°C	50°C ± 2 °C
Cooler			°C	(-)-3 °C ± 2 °C
Converter			°C	325 °C ± 5 °C
Converter Set			°C	325 °C
<b>Pressure</b>			mmHg	250 ± 100 mmHg
<b>Flow</b>			L/min	0.5 to 1.00 L/min

Note :



บริษัท คิว-ซี โซลูชันส์ จำกัด

7/409 ซอยวิภาวดีรังสิต 36 ถนนวิภาวดีรังสิต แขวงจตุจักร เขตจตุจักร กรุงเทพฯ 10900

โทรศัพท์ : (662) 939-5711 (12 Lines) โทรสาร : (662) 939-4207-8

Website <http://www.qshe.co.th> E-mail-address: [info@qshe.co.th](mailto:info@qshe.co.th)



SO<sub>2</sub> Analyzer

Equipment : Sulfur Dioxide analyzer.

Model : 43i

Serial Number : 1310957747

Manufacturer : Thermo

Diagnostic test value				
Parameter	Observed value		Unit	Nominal range
	Before	After		
Sample reading			ppb	
Range			ppb	50 to 1000 ppb
Averaging Time			Sec	10 to 300 Sec
Calibration Factors				
SO <sub>2</sub> BKG. ppb			ppb	0 to 60
SO <sub>2</sub> COEF			-	1.0 ± 0.3
Instrument Controls				
Temp Compensation			On/Off	On
Pressure Compensation			On/Off	On
Flash Lamp			On/Off	On
Communication setting				
Baud Rate			bps	9600 to 115000
Instrument ID			-	0 to 99
Screen Contrast			%	0 to 100
Service Mode			On/Off	Up to used
Diagnostics				
Voltages				
Motherboard voltages:				
3.3 Supply			Vdc	3.3 +/- 1 Vdc
5.0 Supply			Vdc	5.0 +/- 1 Vdc
15.0 Supply			Vdc	15.0 +/- 1 Vdc
24.0 Supply			Vdc	24.0 +/- 1 Vdc
-3.3 Supply			Vdc	- 3.3 +/- 1 Vdc
Interface board voltages:				
PMT Supply				
Flash Supply				
3.3 Supply			Vdc	3.3 +/- 1 Vd
5.0 Supply			Vdc	5.0 +/- 1 Vdc
15.0 Supply			Vdc	15.0 +/- 1 Vdc
-15.0 Supply			Vdc	-15.0 +/- 1 Vdc
24.0 Supply			Vdc	24.0 +/- 1 Vdc
Temperatures				
Internal			°C	15°C to 45°C
Chamber			°C	45°C ± 2°C
Pressure			mmHg	750 ± 100 mmHg
Flow			L/min	0.5 to 1.00 L/min
Lamp intensity			%	40 – 100 %

Note : หน้าจอมีด มองไม่ชัดเจน



บริษัท คิว-ชี โซลูชันส์ จำกัด

7/409 ซอยวิภาวดีรังสิต 36 ถนนวิภาวดีรังสิต แขวงจตุจักร เขตจตุจักร กรุงเทพฯ 10900

โทรศัพท์ : (662) 939-5711 (12 Lines) โทรสาร : (662) 939-4207-8

Website <http://www.qshe.co.th> E-mail-address: [info@qshe.co.th](mailto:info@qshe.co.th)

## SINGLE-POINT GAS CALIBRATION

NO<sub>x</sub>, SO<sub>2</sub>, CO Analyzer.

Equipment :	All analyzer.	Model :	42i, 43i,THC
Serial Number :	--	Manufacturer :	Thermo, Horiba

Standard gas concentration			Dilutor detail	
Sulfur Dioxide (SO <sub>2</sub> )	44.44	ppm	Manufacturer :	Thermo
Nitric Oxide (NO)	45.84	ppm	Model :	146i
Methane (CH <sub>4</sub> )	506.7	ppm	Serial number :	1201351404
Carbon Monoxide (CO)	4513	ppm		
Cylinder NO. :	CC507818			
Expiration Date :	13 Aug 2023			

## BEFORE CALIBRATION RESULT

PARAMETER	ZERO			SPAN			JUDGEMENT
	IDEAL	ACTUAL	ERROR	IDEAL	ACTUAL	%ERROR	
NO (ppb)	0.00			400			
NO <sub>x</sub> (ppb)	0.00			400			
SO <sub>2</sub> (ppb)	0.00			400			
CH <sub>4</sub> (ppm)	0.00			4.43			
THC(ppm)	0.00			4.43			

## AFTER CALIBRATION RESULT

PARAMETER	ZERO			SPAN			JUDGEMENT
	IDEAL	ACTUAL	ERROR	IDEAL	ACTUAL	%ERROR	
NO (ppb)	0.00			400			
NO <sub>x</sub> (ppb)	0.00			400			
SO <sub>2</sub> (ppb)	0.00			400			
CH <sub>4</sub> (ppm)	0.00			4.00			
THC(ppm)	0.00			4.00			

Remark:



บริษัท คิว-ชี โซลูชันส์ จำกัด

7/409 ซอยวิภาวดีรังสิต 36 ถนนวิภาวดีรังสิต แขวงจตุจักร เขตจตุจักร กรุงเทพฯ 10900

โทรศัพท์ : (662) 939-5711 (12 Lines) โทรสาร : (662) 939-4207-8

Website <http://www.qshe.co.th> E-mail-address: [info@qshe.co.th](mailto:info@qshe.co.th)

Job Number :	J092500024	Customer Name :	IRPC
Equipment :	AQMs Station.	Contact Name :	KhunWirasakKhumsuk
Model :	AQMs Station.	Telephone Number :	081-803-0475
Serial Number :	Pluak Kate Station	E-mail address/Fax. :	<a href="mailto:wirasak.k@irpc.co.th">wirasak.k@irpc.co.th</a>
Working Date :	08 May 2025	Working Hour :	4 Hours

## Service Report

Working Scope:

Service Station

Physical Checking:

- ตรวจเช็ค Data logger พบว่าทำงานได้ปกติ
- ตรวจเช็ค Diagnostic of all analyzers อยู่ในเกณฑ์ปกติ
- ตรวจเช็ค Reading of all analyzers และ Met sensor พบว่าปกติ
- ตรวจเช็ค ผล Calibration พบว่าอยู่ในเกณฑ์ปกติ
- ตรวจเช็ค Dilutor และ Zero Air พบว่าทำงานได้ปกติ
- ตรวจเช็ค เครื่องวัดฝุ่น PM-10 พบว่าทำงานได้ปกติ
- ตรวจเช็ค เครื่อง THC analyzer พบว่าทำงานได้ปกติ
- ตรวจเช็ค การทำงานของระบบไฟฟ้า และ UPS พบว่าทำงานได้ปกติ
- ทำความสะอาดภายในสถานี และ บริเวณรอบสถานี

Correction working:

Calibrate single-point of all analyzers.	Drain water for pump of Zero Air.
Replace sample filter 47 mm.	

Part Replacements:

- Sample Filter 47 mm. 6 ea. (Part support by IRPC)

Addition Recommended:

- End -

Serviced by :	ชินโรส มุขโรจน์	Serviced Date	08 May 2025
Approved by:		Approved Date :	08 May 2025



บริษัท คิว-ซี โซลูชั่นส์ จำกัด

7/409 ซอยวิภาวดีรังสิต 36 ถนนวิภาวดีรังสิต แขวงจตุจักร เขตจตุจักร กรุงเทพฯ 10900

โทรศัพท์ : (662) 939-5711 (12 Lines) โทรสาร : (662) 939-4207-8

Website <http://www.qshe.co.th> E-mail-address: [info@qshe.co.th](mailto:info@qshe.co.th)



## General Checking

Equipment :	AQMs Pluak Kate	Model :	-
Serial Number :	Pluak Kate Station	Manufacturer :	-

Item	Description	Set-Point Value	Status & Value	Remark
	<u>On Mobile</u>			
1	Air conditioner operation	OK	OK	
2	Mobile temperature	25-27 °C	26°C	
3	Lighting system	OK	OK	
4	Lamp in sampling box	OK	OK	
5	Sampling probe	Clean	Clean	
6	Blower	OK	OK	
7	Drain liquid in tank	Drain	Drain	
8	Compressor tank set pressure	80 psi	80 psi	
9	Zero air compressor operation	OK	OK	
10	Silica gel for dry air of NO <sub>x</sub> analyzer	OK	OK	
11	UPS 3 KVA	OK	OK	
12	Data logger	OK	OK	
13	Ventilation fan	OK	OK	
14	Power cable	OK	OK	
15	Hydrogen Gas	-	1500/40 psi	
16	Standard gas#1 (NO,SO <sub>2</sub> ,HC,CO)	-	1900/32 psi	

Note :



บริษัท คิว-ซี โซลูชั่นส์ จำกัด

7/409 ซอยวิภาวดีรังสิต 36 ถนนวิภาวดีรังสิต แขวงจตุจักร เขตจตุจักร กรุงเทพฯ 10900

โทรศัพท์ : (662) 939-5711 (12 Lines) โทรสาร : (662) 939-4207-8

Website <http://www.qshe.co.th> E-mail-address: [info@qshe.co.th](mailto:info@qshe.co.th)

NO-NO<sub>2</sub>-NO<sub>x</sub> Analyzer

Equipment :	NO-NO <sub>2</sub> -NO <sub>x</sub> analyzer.	Model :	42i
Serial Number :	1170530044	Manufacturer :	Thermo Scientific

Diagnostic test value				
Parameter	Observed value		Unit	Nominal range
	Before	After		
Sample reading				
NO reading	0.5	1.3	ppb	
NO <sub>x</sub> reading	4.2	4.1	ppb	
Range	500	500	ppb	50 to 1000 ppb
Averaging Time	30	30	Sec	10 to 300 Sec
Calibration Factors				
NO BKG. ppb	12.2	12.3	ppb	0 to 60
NO <sub>x</sub> BKG. ppb	12.2	12.3	ppb	0 to 60
NO COEF.	0.957	0.957	-	1.0 ± 0.3
NO <sub>x</sub> COEF.	1.000	1.000	-	1.0 ± 0.3
NO <sub>2</sub> COEF.	1.000	1.000	-	1.0 ± 0.3
Instrument Controls				
Ozonator	On	On		On/Off
PMT Supply	On	On		On/Off
Auto/Manual Mode	NO/NO <sub>x</sub>	NO/NO <sub>x</sub>		NO/NO <sub>x</sub> , NO, NO <sub>x</sub>
Baud Rate	9600	9600	bps	1200 to 9600
Temp Compensation	On	On	-	On/Off
Pressure Compensation	On	On	-	On/Off
Screen Contrast	45	45	%	0 to 100
Service Mode	Off	Off	-	On/Off, Up to used
Diagnostics				
Voltages				
PMT Supply	-917.6	-917.6	Vdc	-400 to -1200 Vdc
5 Supply	4.9	4.9	Vdc	5.0 ± 1 Vdc
15 Supply	15.1	15.1	Vdc	15.0 ± 1 Vdc
-15 Supply	-15.0	-15.0	Vdc	-15.0 ± 1 Vdc
Temperatures				
Internal	34.3	35.8	°C	15 °C to 45 °C
Chamber	49.7	50.0	°C	50°C ± 2 °C
Cooler	-3.0	-3.0	°C	(-)3 °C ± 2 °C
Converter	323.4	325.5	°C	325 °C ± 5 °C
Converter Set	325.0	325.0	°C	325 °C
Pressure	224.9	241.8	mmHg	250 ± 100 mmHg
Flow	0.497	0.637	L/min	0.5 to 1.00 L/min

Note :



บริษัท คิว-ชี โซลูชั่นส์ จำกัด

7/409 ซอยวิภาวดีรังสิต 36 ถนนวิภาวดีรังสิต แขวงจตุจักร เขตจตุจักร กรุงเทพฯ 10900

โทรศัพท์ : (662) 939-5711 (12 Lines) โทรสาร : (662) 939-4207-8

Website <http://www.qshe.co.th> E-mail-address: [info@qshe.co.th](mailto:info@qshe.co.th)

SO<sub>2</sub> Analyzer

Equipment : Sulfur Dioxide analyzer.

Model : 43I-BZSAB

Serial Number : CM06280010

Manufacturer : Thermo Scientific

Diagnostic test value				
Parameter	Observed value		Unit	Nominal range
	Before	After		
Sample reading	0.1	0.9	ppb	
Range	500	500	ppb	50 to 1000 ppb
Averaging Time	30	30	Sec	10 to 300 Sec
Calibration Factors				
SO <sub>2</sub> BKG. ppb	28.3	24.1	ppb	0 to 60
SO <sub>2</sub> COEF	0.974	0.974	-	1.0 ± 0.3
Instrument Controls				
Temp Correction	On	On	On/Off	On
Pressure Correction	On	On	On/Off	On
Flash Lamp	On	On	On/Off	On
Communication setting				
Baud Rate	9600	9600	bps	9600 to 115000
Instrument ID	43	43	-	0 to 99
Screen Brightness	50	50	%	0 to 100
Service Mode	Off	Off	On/Off	Up to used
Diagnostics				
Voltages				
Motherboard voltages:				
3.3 Supply	3.3	3.3	Vdc	3.3 +/- 1 Vdc
5.0 Supply	5.0	5.0	Vdc	5.0 +/- 1 Vdc
15.0 Supply	15.1	15.1	Vdc	15.0 +/- 1 Vdc
24.0 Supply	23.9	23.9	Vdc	24.0 +/- 1 Vdc
-3.3 Supply	-3.2	-3.2	Vdc	- 3.3 +/- 1 Vdc
Interface board voltages:				
PMT Supply	-602.0	-602.0		
Flash Supply	825	823		
3.3 Supply	3.3	3.3	Vdc	3.3 +/- 1 Vdc
5.0 Supply	5.0	5.0	Vdc	5.0 +/- 1 Vdc
15.0 Supply	14.7	14.7	Vdc	15.0 +/- 1 Vdc
-15.0 Supply	-15.0	-15.0	Vdc	-15.0 +/- 1 Vdc
24.0 Supply	23.9	23.9	Vdc	24.0 +/- 1 Vdc
Temperatures				
Internal	34.9	35.9	°C	15°C to 45°C
Chamber	45.2	45.2	°C	45°C ± 2°C
Pressure	597.9	725.5	mmHg	750 ± 100 mmHg
Flow	0.624	0.624	L/min	0.5 to 1.00 L/min
Lamp intensity	93	91	%	40 – 100 %

Note :



บริษัท คิว-ชี โซลูชั่นส์ จำกัด

7/409 ซอยวิภาวดีรังสิต 36 ถนนวิภาวดีรังสิต แขวงจตุจักร เขตจตุจักร กรุงเทพฯ 10900

โทรศัพท์ : (662) 939-5711 (12 Lines) โทรสาร : (662) 939-4207-8

Website <http://www.qshe.co.th> E-mail-address: [info@qshe.co.th](mailto:info@qshe.co.th)



## SINGLE-POINT GAS CALIBRATION

All analyzer.

Equipment :	All analyzer.	Model :	42C, 43i , 48i, 49i
Serial Number :	0504710413,CM06280010, 1201351403,CM09040067	Manufacturer :	Thermo

Standard gas concentration			Dilutor detail	
Sulfur Dioxide (SO <sub>2</sub> )	44.7	ppm	Manufacturer :	Thermo
Nitric Oxide (NO)	45.0	ppm	Model :	146C
Methane (CH <sub>4</sub> )	498	ppm	Serial number :	0504710414
Carbon oxide (CO)	4550	ppm		
Cylinder NO. :	A00931SK			
Expiration Date :	8 Sep 2026			

## BEFORE CALIBRATION RESULT

PARAMETER	ZERO			SPAN			JUDGEMENT
	IDEAL	ACTUAL	ERROR	IDEAL	ACTUAL	%ERROR	
NO (ppb)	0.00			400			
NO <sub>x</sub> (ppb)	0.00			400			
SO <sub>2</sub> (ppb)	0.00			400			
CO (ppm)	0.00			40.3			
O <sub>3</sub> (ppb)	0.00			400			
CH <sub>4</sub> (ppm)	0.00			5.00			
THC (ppm)	0.00			5.00			

## AFTER CALIBRATION RESULT

PARAMETER	ZERO			SPAN			JUDGEMENT
	IDEAL	ACTUAL	ERROR	IDEAL	ACTUAL	%ERROR	
NO (ppb)	0.00	1.0	1.00	400	399.0	-0.25	Valid
NO <sub>x</sub> (ppb)	0.00	1.5	1.50	400	401.0	0.25	Valid
SO <sub>2</sub> (ppb)	0.00	1.0	1.00	400	403.0	0.75	Valid
CO (ppm)	0.00	0.15	0.15	40.3	40.2	-0.25	Valid
O <sub>3</sub> (ppb)	0.00	1.0	1.00	400	401.0	0.25	Valid
CH <sub>4</sub> (ppm)	0.00			5.00			
THC (ppm)	0.00			5.00			

Remark :



บริษัท คิว-ชี โซลูชันส์ จำกัด

7/409 ซอยวิภาวดีรังสิต 36 ถนนวิภาวดีรังสิต แขวงจตุจักร เขตจตุจักร กรุงเทพฯ 10900

โทรศัพท์ : (662) 939-5711 (12 Lines) โทรสาร : (662) 939-4207-8

Website <http://www.qshe.co.th> E-mail-address: [info@qshe.co.th](mailto:info@qshe.co.th)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด  
S.P.S. CONSULTING SERVICE CO., LTD.  
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900  
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900  
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

CALIBRATION REPORT						
SO <sub>2</sub> FLUORESCENT ANALYZER						
DATE :	18 May 2025	BRAND :	API	MODEL :	100A	
NO.	SO <sub>2</sub> -B01	SERIAL NO.	1749			
Calibrator (Dilution System)						
Brand	: Teledyne			Model	: 700	
Last Cal. Date	: 29 October 2024			Serial No.	: 421	
Reference Standard Gas						
Standard Gas	: Sulphur Dioxide (SO <sub>2</sub> )			Cylinder No.	: A00814SK	
Certified Date	: 21 June 2021	Expired Date	: 21 June 2029	Cylinder Conc.	: 49.8 ppm	
CALIBRATING CONDITION						
Pressure	1011	mmbar	Temp.	24.5	°C	
% RH						50
CALIBRATION SETTING						
Span	Initial Reading (Before Adj.),PPB			Final Reading (After Adj.),PPB		
Set Point	Expected Concentration	Analyzer Response	%Dif	Analyzer Response	Slope	
Zero	0	0.10	-	0	-	
SO <sub>2</sub> Span	400.0	399.7	-0.075	400.0	1.006	
API Model 100E SO <sub>2</sub> Analyzer Check list						
Test Values	Observed Value	Units	Nominal Range			
RANGE	500	PPB	0-500			
SAMPLE PRESS	28.5	in-Hg	25-35			
SAMPLE FLOW	659	cc/min	650 ± 10%			
PMT	103.2	mV	-20-150 with Zero Air			
UV LAMP	3024.8	mV	1000-4900			
STR. LGT	61.4	PPB	<100			
DRK PMT	62.9	mV	-50 - 200			
DRK LMP	57.6	mV	-50 - 200			
HVPS	673	V	550-900 constant			
DCPS	2525	mV	2500 ± 200			
RCELL TEMP	50.1	°C	50 ± 1			
BOX TEMP	29.3	°C	5-40			
PMT TEMP	7.0	°C	7 ± 2.0			
SO <sub>2</sub> Span Conc	400	PPB	20-20,000			
SO <sub>2</sub> Slope	1.006	-	1.0 ± 0.3			
SO <sub>2</sub> Offset	21.9	mV	<250			
Stability at Zero	0.1	PPB	<0.2			
Stability at Span	0.2	PPB	0.5% of reading (above 50 ppb)			

Calibrated by :

(Mr.Kaseam Simaphon)

Approved by :

(Mr.Yuthana Thanataranit)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด  
S.P.S. CONSULTING SERVICE CO., LTD.  
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจตุจักร เขตจตุจักร กรุงเทพฯ 10900  
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900  
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

CALIBRATION REPORT					
SO <sub>2</sub> FLUORESCENT ANALYZER					
DATE :	18 May 2025	BRAND :	API	MODEL :	TML-60
NO.	SO <sub>2</sub> -R08	SERIAL NO.	TRS1064		
Calibrator (Dilution System)					
Brand	: Teledyne		Model	: 700	
Last Cal. Date	: 29 October 2024		Serial No.	: 421	
Reference Standard Gas					
Standard Gas	: Sulphur Dioxide (SO <sub>2</sub> )		Cylinder No.	: A00814SK	
Certified Date	: 21 June 2021	Expired Date	: 21 June 2029	Cylinder Conc.	: 49.8 ppm
CALIBRATING CONDITION					
Pressure	1011	mmbar	Temp.	24.5	°C
% RH	50				
CALIBRATION SETTING					
Span	Initial Reading (Before Adj.),PPB			Final Reading (After Adj.),PPB	
Set Point	Expected Concentration	Analyzer Response	%Dif	Analyzer Response	Slope
Zero	0	-0.10	-	0	-
SO <sub>2</sub> Span	400.0	399.9	-0.025	400.0	1.009
API Model 100E SO <sub>2</sub> Analyzer Check list					
Test Values	Observed Value	Units	Nominal Range		
RANGE	500	PPB	0-500		
SAMPLE PRESS	28.7	in-Hg	25-35		
SAMPLE FLOW	654	cc/min	650 ± 10%		
PMT	103.3	mV	-20-150 with Zero Air		
UV LAMP	3030.9	mV	1000-4900		
STR. LGT	61.8	PPB	<100		
DRK PMT	63.3	mV	-50 - 200		
DRK LMP	58.1	mV	-50 - 200		
HVPS	672	V	550-900 constant		
DCPS	2517	mV	2500 ± 200		
RCELL TEMP	50.0	°C	50 ± 1		
BOX TEMP	28.8	°C	5-40		
PMT TEMP	7.2	°C	7 ± 2.0		
SO <sub>2</sub> Span Conc	400	PPB	20-20,000		
SO <sub>2</sub> Slope	1.009	-	1.0 ± 0.3		
SO <sub>2</sub> Offset	21.8	mV	<250		
Stability at Zero	0.1	PPB	<0.2		
Stability at Span	0.2	PPB	0.5% of reading (above 50 ppb)		

Calibrated by :

(Mr.Kaseam Simaphon)

Approved by :

(Mr.Yuthana Thanataranit)





บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด  
S.P.S. CONSULTING SERVICE CO., LTD.  
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจตุจักร เขตจตุจักร กรุงเทพฯ 10900  
/ Soi Phaholyothin 24, Phaholyothin Rd., Jomjod, Chaluchak, Bangkok 10900  
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscn.com, www.spscn.com

CALIBRATION REPORT						
SO <sub>2</sub> FLUORESCENT ANALYZER						
DATE :	18 May 2025	BRAND :	API	MODEL :	100E	
NO.	SO <sub>2</sub> -R09	SERIAL NO.	76			
Calibrator (Dilution System)						
Brand : Teledyne			Model : 700			
Last Cal. Date : 29 October 2024			Serial No. : 421			
Reference Standard Gas						
Standard Gas : Sulphur Dioxide (SO <sub>2</sub> )			Cylinder No. : A008145K			
Certified Date : 21 June 2021		Expired Date : 21 June 2029		Cylinder Conc. : 49.8 ppm		
CALIBRATING CONDITION						
Pressure	1011	mmbar	Temp.	24.6	°C	
% RH						48
CALIBRATION SETTING						
Span	Initial Reading (Before Adj.),PPB			Final Reading (After Adj.),PPB		
Set Point	Expected Concentration	Analyzer Response	%Dif	Analyzer Response	Slope	
Zero	0	0.10	-	0	-	
SO <sub>2</sub> Span	400.0	399.7	-0.075	400.0	1.006	
API Model 100E SO <sub>2</sub> Analyzer Check list						
Test Values	Observed Value	Units	Nominal Range			
RANGE	500	PPB	0-500			
SAMPLE PRESS	28.5	in-Hg	25-35			
SAMPLE FLOW	653	cc/min	650 ± 10%			
PMT	103.2	mV	-20-150 with Zero Air			
UV LAMP	319.5	mV	1000-4900			
STR. LGT	61.6	PPB	<100			
DRK PMT	63.1	mV	-50 - 200			
DRK LMP	57.7	mV	-50 - 200			
HVPS	673	V	550-900 constant			
DCPS	2528	mV	2500 ± 200			
RCELL TEMP	50.1	°C	50 ± 1			
BOX TEMP	29.3	°C	5-40			
PMT TEMP	7.0	°C	7 ± 2.0			
SO <sub>2</sub> Span Conc	400	PPB	20-20,000			
SO <sub>2</sub> Slope	1.006	-	1.0 ± 0.3			
SO <sub>2</sub> Offset	21.9	mV	<250			
Stability at Zero	0.1	PPB	<0.2			
Stability at Span	0.2	PPB	0.5% of reading (above 50 ppb)			

Calibrated by :

*Mr. Kaseam Simaphon*

(Mr.Kaseam Simaphon)

Approved by :

*Mr. Yuthana Thanataranit*

(Mr.Yuthana Thanataranit)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด

S.P.S. CONSULTING SERVICE CO., LTD.

7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900  
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chaluchak, Bangkok 10900  
Tel : (662) 939-4370-72. Fax : (662) 513-4221. E-mail : sale@spscon.com. www.spscon.com

CALIBRATION REPORT						
CHEMILUMINESCENT NO / NO <sub>2</sub> / NO <sub>x</sub> ANALYZER						
DATE :	18 May 2025	BRAND :	API	MODEL :	200E	
NO.	NOX-B06	SERIAL NO.	2286			
Calibrator (Dilution System)						
Brand	: Teledyne			Model	: 700	
Last Cal. Date	: 29 October 2024			Serial No.	: 421	
Reference Standard Gas						
Standard Gas	: Nitric Oxide (NO)			Cylinder No.	: A00726SV	
Certified Date	: 05 January 2023	Expired Date	: 05 January 2026	Cylinder Conc.	: 48.8 ppm	
CALIBRATING CONDITION						
Pressure	1011	mmbar	Temp.	24.6	°C	
% RH						48
CALIBRATION SETTING						
Span	Initial Reading (Before Adj.),PPB			Final Reading (After Adj.),PPB		
Set Point	Expected Concentration	Analyzer Response	%Dif	Analyzer Response	Slope	
Zero	0	0.11	-	0	-	
NO Span	400	400.2	0.050	400.0	1.010	
NO <sub>x</sub> Span	400	400.3	0.075	400.0	1.014	
API Model 200E NO <sub>x</sub> Analyzer Check List						
Test Values	Observed Value	Units	Nominal Range			
RANGE	500	PPB	500 standard			
STABILITY (Zero Gas)	0.1	PPB	< 2 with zero air			
SAMPLE FLOW	512	cc/min	500 ± 50			
OZONE FLOW	79	cc/min	80 ± 15			
PMT	103.4	mV	-20 - 150			
AZERO	94.1	mV	-20 - 150			
HVPS	673	V	420 - 900 constant			
RCELL TEMP	50.0	°C	50 ± 1			
BOX TEMP	28.8	°C	8 - 48			
PMT TEMP	7.1	°C	7 ± 2			
MOLY TEMP	315.2	°C	315 ± 5			
RCELL PRESS	8.3	IN-Hg-A	2 - 10 constant			
SAMPLE PRESS	28.5	IN-Hg-A	25 - 30 constant			
NO Span Conc	400	PPB	20 - 20,000			
NO <sub>x</sub> Span Conc	400	PPB	20 - 20,000			
NO Slope	1.010	-	1.0 ± 0.3			
NO <sub>x</sub> Slope	1.024	-	1.0 ± 0.3			
NO Offset	1.8	mV	-20 to +150			
NO <sub>x</sub> Offset	1.1	mV	-20 to 150			
Stability at Zero	0.1	PPB	< 0.2			
Stability at Span	0.2	PPB	< 2 ppb @ 400 ppb span gas			

Calibrated by :

*Mr. Kaseam Simaphon*

(Mr.Kaseam Simaphon)

Approved by :

*Mr. Yuthana Thanataranit*

(Mr.Yuthana Thanataranit)





บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด  
S.P.S. CONSULTING SERVICE CO., LTD.  
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจตุจักร เขตจตุจักร กรุงเทพฯ 10900  
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900  
Tel : (662) 939-1370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

CALIBRATION REPORT					
CHEMILUMINESCENT NO / NO <sub>2</sub> / NO <sub>x</sub> ANALYZER					
DATE :	18 May 2025	BRAND :	API	MODEL :	200E
NO.	NOX-B09	SERIAL NO.	4412		
Calibrator (Dilution System)					
Brand	: Teledyne		Model	: 700	
Last Cal. Date	: 29 October 2024		Serial No.	: 421	
Reference Standard Gas					
Standard Gas	: Nitric Oxide (NO)		Cylinder No.	: A00726SV	
Certified Date	: 05 January 2023		Expired Date	: 05 January 2026	
			Cylinder Conc.	: 48.8 ppm	
CALIBRATING CONDITION					
Pressure	1011	mmbar	Temp.	24.5	°C
			% RH	50	
CALIBRATION SETTING					
Span	Initial Reading (Before Adj.), PPB			Final Reading (After Adj.), PPB	
Set Point	Expected Concentration	Analyzer Response	% Dif	Analyzer Response	Slope
Zero	0	0.11	-	0	-
NO Span	400	400.1	0.025	400.0	1.010
NO <sub>x</sub> Span	400	400.3	0.075	400.0	1.014
API Model 200E NO <sub>x</sub> Analyzer Check List					
Test Values	Observed Value	Units	Nominal Range		
RANGE	500	PPB	500 standard		
STABILITY (Zero Gas)	0.1	PPB	< 2 with zero air		
SAMPLE FLOW	510	cc/min	500 ± 50		
OZONE FLOW	79	cc/min	80 ± 15		
PMT	103.2	mV	-20 - 150		
AZERO	93.9	mV	-20 - 150		
HVPS	675	V	420 - 900 constant		
RCELL TEMP	50.2	°C	50 ± 1		
BOX TEMP	29.1	°C	8 - 48		
PMT TEMP	7.3	°C	7 ± 2		
MOLY TEMP	315.2	°C	315 ± 5		
RCELL PRESS	8.4	IN-Hg-A	2 - 10 constant		
SAMPLE PRESS	28.6	IN-Hg-A	25 - 30 constant		
NO Span Conc	400	PPB	20 - 20,000		
NO <sub>x</sub> Span Conc	400	PPB	20 - 20,000		
NO Slope	1.010	-	1.0 ± 0.3		
NO <sub>x</sub> Slope	1.014	-	1.0 ± 0.3		
NO Offset	1.5	mV	-20 to +150		
NO <sub>x</sub> Offset	0.9	mV	-20 to 150		
Stability at Zero	0.1	PPB	< 0.2		
Stability at Span	0.2	PPB	< 2 ppb @ 400 ppb span gas		

Calibrated by :

(Mr.Kaseam Simaphon)

Approved by :

(Mr.Yuthana Thanataranit)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด  
S.P.S. CONSULTING SERVICE CO., LTD.  
7 ซอยพลอยอิน 24 ถนนพลอยอิน แขวงจตุจักร กรุงเทพฯ 10900  
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900  
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

CALIBRATION REPORT					
CHEMILUMINESCENT NO / NO <sub>2</sub> / NO <sub>x</sub> ANALYZER					
DATE :	18 May 2025	BRAND :	API	MODEL :	200A
NO.	NOX-B17	SERIAL NO.	1977		
Calibrator (Dilution System)					
Brand	: Teledyne		Model	: 700	
Last Cal. Date	: 29 October 2024		Serial No.	: 421	
Reference Standard Gas					
Standard Gas	: Nitric Oxide (NO)		Cylinder No.	: A007265V	
Certified Date	: 05 January 2023		Expired Date	: 05 January 2026	
			Cylinder Conc.	: 48.8 ppm	
CALIBRATING CONDITION					
Pressure	1011	mmbar	Temp.	24.5	°C
			% RH	50	
CALIBRATION SETTING					
Span	Initial Reading (Before Adj.), PPB			Final Reading (After Adj.), PPB	
Set Point	Expected Concentration	Analyzer Response	%Dif	Analyzer Response	Slope
Zero	0	0.10	-	0	-
NO Span	400	399.7	-0.075	400.0	106.000
NO <sub>x</sub> Span	400	400.1	0.025	400.0	1.010
API Model 200E NO <sub>x</sub> Analyzer Check List					
Test Values	Observed Value	Units	Nominal Range		
RANGE	500	PPB	500 standard		
STABILITY (Zero Gas)	0.1	PPB	< 2 with zero air		
SAMPLE FLOW	504	cc/min	500 ± 50		
OZONE FLOW	78	cc/min	80 ± 15		
PMT	102.9	mV	-20 - 150		
AZERO	93.8	mV	-20 - 150		
HVPS	674	V	420 - 900 constant		
RCCELL TEMP	50.3	°C	50 ± 1		
BOX TEMP	29.2	°C	8 - 48		
PMT TEMP	7.4	°C	7 ± 2		
MOLY TEMP	315.1	°C	315 ± 5		
RCCELL PRESS	8.2	IN-Hg-A	2 - 10 constant		
SAMPLE PRESS	28.5	IN-Hg-A	25 - 30 constant		
NO Span Conc	400	PPB	20 - 20,000		
NO <sub>x</sub> Span Conc	400	PPB	20 - 20,000		
NO Slope	1.006	-	1.0 ± 0.3		
NO <sub>x</sub> Slope	1.010	-	1.0 ± 0.3		
NO Offset	1.1	mV	-20 to +150		
NO <sub>x</sub> Offset	0.7	mV	-20 to 150		
Stability at Zero	0.1	PPB	< 0.2		
Stability at Span	0.2	PPB	< 2 ppb @ 400 ppb span gas		

Calibrated by :

(Mr.Kaseam Simaphon)

Approved by :

(Mr.Yuthana Thanataranit)

ลำดับที่ 2

คุณภาพอากาศจากแหล่งกำเนิด



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด  
S.P.S. CONSULTING SERVICE CO., LTD.  
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900  
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900  
Tel : (662) 939-4370-72. Fax : (662) 513-4221. E-mail : sale@spscon.com.. www.spscon.com

## Console Calibration Report

Calibration Method

Critical Orifices

### Calibration Data

Console Data		Calibration Data		
No.	Serial No.	Date	y	DH <sub>g</sub> (mmH <sub>2</sub> O)
B01	1563	03/03/2025	1.003	49.40
B02	8002514	03/03/2025	1.004	49.57
B03	1503016	04/03/2025	0.999	49.93
B04	00006659	04/03/2025	0.996	49.88
B05	00007428	04/03/2025	1.007	49.14
R01	1561	05/03/2025	0.996	49.32
R02	8002513	04/03/2025	1.003	49.96
R03	1570	04/03/2025	0.998	50.08
R04	8002519	03/03/2025	0.997	49.53
R05	1503015	05/03/2025	1.005	50.25

Remark : Accept Value of y (test) is  $0.97 < y < 1.03$

Accept Value of DH<sub>g</sub> (test) is  $46.7 \pm 6.4$  (mmH<sub>2</sub>O)

Calibrated by :

Adul Dangklom  
(Mr. Adul Dangklom)

Approved by :

Peera Detudom  
(Mr. Peera Detudom)





บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด  
S.P.S. CONSULTING SERVICE CO., LTD.  
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900  
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900  
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com., www.spscon.com

## Pitot Tube Calibration Report

Calibration Method

Standard Pitot Tube

### Calibration Data

Pitot Tube Data			Calibration Data		
No.	Type of Pitot	Coefficient of Standard Pitot	Date	Avg. of Cp (test)	
				Side A	Side B
B03	S	0.99	01/05/2025	0.84	0.83
B04	S	0.99	01/05/2025	0.84	0.84
B05	S	0.99	01/05/2025	0.85	0.84
B07	S	0.99	01/05/2025	0.84	0.83
B08	S	0.99	01/05/2025	0.85	0.84
B09	S	0.99	02/05/2025	0.83	0.84
B11	S	0.99	01/05/2025	0.84	0.85
B16	S	0.99	01/05/2025	0.84	0.84
B18	S	0.99	01/05/2025	0.84	0.83
B19	S	0.99	01/05/2025	0.85	0.84
B21	S	0.99	02/05/2025	0.84	0.84
B24	S	0.99	05/05/2025	0.85	0.84
B27	S	0.99	05/05/2025	0.85	0.84
B30	S	0.99	05/05/2025	0.84	0.85
B31	S	0.99	05/05/2025	0.84	0.84
B33	S	0.99	01/05/2025	0.84	0.85
B35	S	0.99	01/05/2025	0.84	0.84

Remark : Accept value of Cp (test) is  $0.84 \pm 0.01$

Calibrated by :

Adul Dangklom  
(Mr. Adul Dangklom)

Approved by :

Peera Detudom  
(Mr. Peera Detudom)





บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด

S.P.S. CONSULTING SERVICE CO., LTD.

7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900

7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900

Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

## Pitot Tube Calibration Report

Calibration Method

Standard Pitot Tube

### Calibration Data

Pitot Tube Data			Calibration Data		
No.	Type of Pitot	Coefficient of Standard Pitot	Date	Avg. of Cp (test)	
				Side A	Side B
B36	S	0.99	01/05/2025	0.84	0.84
B37	S	0.99	01/05/2025	0.84	0.83
B38	S	0.99	01/05/2025	0.85	0.84
B39	S	0.99	01/05/2025	0.85	0.84
B40	S	0.99	01/05/2025	0.84	0.83
B41	S	0.99	01/05/2025	0.85	0.84
B44	S	0.99	01/05/2025	0.84	0.84
B45	S	0.99	02/05/2025	0.84	0.84
B46	S	0.99	02/05/2025	0.84	0.83
B47	S	0.99	02/05/2025	0.83	0.84
B48	S	0.99	02/05/2025	0.85	0.84
B49	S	0.99	01/05/2025	0.84	0.84
B54	S	0.99	01/05/2025	0.84	0.85
B56	S	0.99	01/05/2025	0.85	0.84
B57	S	0.99	01/05/2025	0.84	0.84
B58	S	0.99	05/05/2025	0.83	0.84

Remark : Accept value of Cp (test) is  $0.84 \pm 0.01$

Calibrated by :

Adul Dangklom  
(Mr. Adul Dangklom)

Approved by :

Peera Detudom  
(Mr. Peera Detudom)



CERTIFICATE No : 25M2254

REFERENCE No : 76365-1

PAGE : 1 OF 2

## Certificate of Calibration

**EQUIPMENT** : DIGITAL BALANCE

**MANUFACTURER** : METTLER TOLEDO

**MODEL** : XS105DU

**SERIAL No** : 1126422905

**ID No** : BA05/50

**CONDITION AS RECEIVED** : USED ITEM

**SUBMITTED BY** : S.P.S. CONSULTING SERVICE CO., LTD.  
7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN RD.,  
JOMPOL, CHATUCHAK, BANGKOK 10900

**CALIBRATED BY** : ATSAWIN Y.

**CALIBRATION DATE** : 07-Mar-25

**APPROVED BY** :   
PONGSAK J.

**ISSUED DATE** : 13-Mar-25

**RECEIVED DATE** : 07-Mar-25

THIS CERTIFICATE MAY NOT BE REPRODUCED OTHER THAN IN FULL EXCEPT WITH THE PRIOR WRITTEN APPROVAL OF  
QUALITY CALIBRATION CO., LTD.







CERTIFICATE No : 25M2254

PAGE : 2 OF 2

## Calibration Report

EQUIPMENT : DIGITAL BALANCE MODEL : XS105DU  
MANUFACTURER : METTLER TOLEDO S/N : 1126422905  
ID No : BA05/50 RECEIVED DATE : 07-Mar-25  
AIR PRESSURE : 1009mbar  $\pm$  1mbar CALIBRATION DATE : 07-Mar-25  
AMBIENT TEMPERATURE : 24°C  $\pm$  1°C RELATIVE HUMIDITY : 54 %RH  $\pm$  10 % RH

### CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED BY ACCORDING TO UKAS LAB 14 EDITION 6:2019 BY USING KNOWN WEIGHT STANDARD WEIGHT. THE BALANCE WAS NOT ADJUSTED BEFORE CALIBRATION. THE BALANCE HAS NO ZERO TRACKING FUNCTION. REPEATABILITY WAS MEASURED BY USING 10 REPEATED MEASUREMENTS. LINEARITY WAS MEASURED COVERING 10 POINTS, EVENLY SPREAD OVER THE RANGE. THE INSTRUMENT WAS SET ZERO BEFORE PERFORMING THE LINEARITY TEST. OFF-CENTER LOADING WAS MEASURED BY USING STANDARD WEIGHTS PLACED ON THE PAN AND MOVED TO VARIOUS POSITIONS ON THE PAN.

### 2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) STANDARD WEIGHT SET	E2	QK-I-151	C02250116	28-Jan-27
2) STANDARD WEIGHT	E2	15843	C02250117	29-Jan-27

3. THE CERTIFICATE IS VALID FOR THE ITEM CALIBRATED AS SHOWN ON THE DATE AND PLACE OF CALIBRATION ONLY.

4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.

5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-

- NATIONAL INSTITUTE OF METROLOGY (THAILAND)

### RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

1. ZERO SETTING FUNCTION : NORMAL


2. TARE FUNCTION : NORMAL

3. REPEATABILITY OF READING AT 120 g WAS 0.000055 g

4. DEPARTURE FROM NOMINAL VALUE/ LINEARITY

NOMINAL VALUE (g)	BALANCE READING (g)	CORRECTION (g)	UNCERTAINTY ( $\pm$ g)
0.00	0.00000	0.00000	0.000065
0.02	0.01999	0.00001	0.000065
0.10	0.10001	-0.00001	0.000066
0.20	0.20001	-0.00001	0.000066
0.50	0.50002	-0.00002	0.000065
1.00	1.00003	-0.00003	0.000066
2.00	2.00001	-0.00001	0.000067
5.00	5.00002	-0.00002	0.000068
10.00	10.00000	0.00000	0.000070
20.00	20.00004	-0.00004	0.000078
50.00	50.00000	0.00000	0.00013
100.00	100.0001	-0.0001	0.00019
120.00	120.0002	-0.0002	0.00022

### 5. OFF CENTER LOADING ERROR



POINT	READING (g)
1	50.0000
2	50.0000
3	50.0000
4	50.0000
5	50.0000
OFF-CENTER LOADING	0.0000

NOTE: THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR  $k=2$ , PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT





## CERTIFICATE OF CALIBRATION FOR

NOMENCLATURE : VACUUM GAUGE  
MANUFACTURER : HI-LIGHT  
MODEL / TYPE : N/A  
SERIAL NO. : N/A[64-220066-2]  
CLID. NO. : 212201113  
JOB CONTROL NO. : 240730078440  
CALIBRATION SERVICE : ☒ IN-LABORATORY ☐ ON-SITE

CUSTOMER : S.P.S. CONSULTING SERVICE CO., LTD.  
7 SOI PHAHOLYOTHIN 24 ROAD., JOMPOL,  
CHATUCHAK, BANGKOK 10900

DATE OF RECEIVED : 30 July 2024

DATE OF ISSUED : 02 August 2024

The report of calibration shall not be reproduced except in full without approval of the Calibration Laboratory Co., Ltd.

Calibrated By : Sittipong Pimdee  
Calibration Engineer

Approved By : Mongkol Yotsoontorn  
Authorized Signatory  
02 August 2024



This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to the International System of Units (SI)

Certificate No. Q24078440

F3-011-05/12-23

page 1 of 3



@clccalibration



# CALIBRATION LABORATORY Co., LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230  
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



## REPORT OF CALIBRATION

### FOR

NOMENCLATURE	:	VACUUM GAUGE
MANUFACTURER	:	HI-LIGHT
MODEL / TYPE	:	N/A
SERIAL NO.	:	N/A[64-220066-2]
DATE OF CALIBRATION	:	31 July 2024
DUE DATE OF CALIBRATION	:	31 July 2025

#### ENVIRONMENT CONDITIONS :

Temperature :  $(23 \pm 2) ^\circ\text{C}$

Relative Humidity :  $(55 \pm 10) \% \text{RH}$

#### PROCEDURE USED :

This instrument was calibrated under procedure No. **CLC-CPPP-05** according to **DKD-R 6-1** as calibration guidelines.

The calibration was performed by direct measurement with Document Process Calibrator and Pressure Module which maintained by the Calibration Laboratory Co., Ltd.

#### REFERENCE STANDARD USED :

Document Process Calibrator, Fluke Model 741B S/N. 8295020 with Pressure Module Model 700PD5 S/N. 89404505.

#### TRACEABILITY :

The measurements are traceable to International System of Units (SI), through National Institute of Metrology (Thailand).  
Certificate No. MP-0040-24, Due Date 08 February 2025.

#### UNCERTAINTY :

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor of  $k = 2$ . It has been evaluated according to the "Calibration of Pressure Gauges (DKD-R 6-1)" which provides a level of confidence approximately 95%.

Certificate No. Q24078440

F3-011-05/12-23

page 2 of 3



@clccalibration



**CONDITION OF CALIBRATION ITEM : RECEIVED IN GOOD OPERATIONAL CONDITION**

**MEASUREMENT RESULTS : ( X ) without adjustment ( ) adjustment**

The DUC was exercised by applying a known pressure from its zero to full scale 1 times. Then 2 series of known gauge pressure were applied. The STD reading were recorded and the means value were reported in the table below.

## CALIBRATION DATA

### **CORRECTION OF PRESSURE**

DUC Test point ( inHg )	STD Reading ( kPa )		Conversion to inHg		Correction ( inHg )	
	Up	Down	Up	Down	Up	Down
0	0.000	0.000	0.0	0.0	0.0	0.0
-5	-16.591	-16.930	-4.9	-5.0	+0.1	0.0
-10	-33.521	-33.521	-9.9	-9.9	+0.1	+0.1
-15	-50.113	-50.113	-14.8	-14.8	+0.2	+0.2
-20	-66.704	-67.043	-19.7	-19.8	+0.3	+0.2
-25	-83.634	-83.973	-24.7	-24.8	+0.3	+0.2
-30	-100.564	-100.564	-29.7	-29.7	+0.3	+0.3

Uncertainty of measurement  $\pm 0.2$  inHg

Transmitting fluid : Air.

Technical Note. Conversion factor 1 kPa ; 0.2953003 inHg

Note. The Scope of Accredited ANAB Certificate No. ACDM-2814 Version 012 Page 43 of 67

**This report is valid for the above stated instrument/s only.**

**### End of Certificate ###**

Certificate No. Q24078440

F3-011-05/12-23

page 3 of 3



**Cert. No. : SP24020**

**Pages 1 of 3**

## Calibration Certificate

**Equipment :** UV-VIS SPECTROPHOTOMETER  
**Manufacturer :** PERKINELMER  
**Model :** LAMBDA 25  
**Serial No.:** 501S14123010  
**ID No.:** SP03/58  
**Calibration Mode :** WAVELENGTH ACCURACY  
PHOTOMETRIC ACCURACY

**Condition As Found :** GOOD

**Customer :** S.P.S. CONSULTING SERVICE CO., LTD.  
7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN ROAD,  
CHOMPHON, CHATUCHAK,  
BANGKOK 10900, THAILAND.

**Location :** WET CHEMISTRY LABORATORY IV

**Ambient Temperature :** ( 28.1  $\pm$  5 ) °C  
**Relative Humidity :** ( 47.2  $\pm$  25 ) %

**Received Date :** 27 AUGUST 2024  
**Calibration Date :** 27 AUGUST 2024  
**Date of Issue :** 27 AUGUST 2024

**Calibrated by :**

Nathakorn Pisutpaisan

**Approved by :**

  
( Thanakul Petchurai )

# SITHIPORN ASSOCIATES CO., LTD.

## CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Banglumru, Bangplud, Bangkok, 10700 Thailand  
Tel. +66 2433 8331 Email : calibration@sithiporn.com

SITHIPORN  
associates



Cert. No. : SP24020

Job No. : VC67SP0013

Pages : 2 of 3

### Calibration Method :

This instrument was calibrated by using on-site calibration procedure In-house method : CP-SP-01

The calibration procedure to direct measurement wavelength accuracy by using wavelength standard solution, Photometric accuracy by using absorbance standard filter and absorbance standard solution

The calibration procedure used was based on ASTM E275-01, ASTM E925-02

### Condition of this result of calibration :

#### 1. Certified reference materials

Material	Ref. type	Cell serial No.	Cert. No.	Due Date
Holmium liquid	RM-HL	29706	106864	01/11/2024
Didymium liquid	RM-DL	28912	106905	02/11/2024
Neutral density filter	RM-1N2N3N	13877	106918	03/11/2024
Potassium dichromate solutions	RM-0204060810	14204	106902	02/11/2024
Potassium Iodide solution	-	KI-0701-001	CI-0185-24	14/05/2026

2. This result of calibration was found accurate as shown on date and place of calibration only.

3. This certificate is traceable to the international system of unit maintained at :

3.1 The UK National Physical Laboratory (NPL)

3.2 The National Institute of Standards and Technology, NIST.

### Result of calibration : Wavelength Accuracy

(Without adjustment)

Material	Certified Values of Reference Material (nm)	UUC* Reading (nm)	Error (nm)	Uncertainty $\pm$ (nm)	k Factor
RM-HL	278.13	278.3	0.17	0.16	2.00
	361.25	361.4	0.15	0.16	2.00
	467.82	467.7	-0.12	0.16	2.00
	536.56	536.5	-0.06	0.16	2.00
	640.50	640.4	-0.10	0.16	2.00
RM-DL	740.09	739.9	-0.19	0.16	2.00
	864.94	865.2	0.26	0.16	2.00

UUC\* = Unit Under Calibration

*G. Petch*



# SITHIPORN ASSOCIATES CO., LTD.

## CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbunru, Bangplud, Bangkok, 10700 Thailand  
Tel. +66 2433 8331 Email : calibration@sithiporn.com

SITHIPORN  
associates



Cert. No. : SP24020

Job No. : VC67SP0013

Pages : 3 of 3

### Result of calibration : Photometric Accuracy

(Without adjustment)

Material	Wavelength (nm)	Filter S/N	Nominal Absorbance (A)	Certified Absorbance (A)	UUC* Reading Absorbance (A)	Error (A)	Uncertainty ± (A)	k Factor
Neutral Density glass filter	440.0	29360	1.0	1.0517	1.0550	0.0033	0.0029	2.00
		29914	0.7	0.7445	0.7460	0.0015	0.0029	2.00
		29381	0.5	0.5416	0.5431	0.0015	0.0030	2.00
	546.1	29360	1.0	0.9821	0.9820	-0.0001	0.0028	2.00
		29914	0.7	0.6961	0.6958	-0.0003	0.0028	2.00
		29381	0.5	0.5073	0.5080	0.0007	0.0029	2.00
	590.0	29360	1.0	1.0222	1.0210	-0.0012	0.0028	2.00
		29914	0.7	0.7237	0.7221	-0.0016	0.0029	2.00
		29381	0.5	0.5361	0.5361	0.0000	0.0031	2.00
	635.0	29360	1.0	0.9753	0.9745	-0.0008	0.0028	2.00
		29914	0.7	0.6910	0.6900	-0.0010	0.0029	2.00
		29381	0.5	0.5211	0.5210	-0.0001	0.0032	2.00
Material	Wavelength (nm)	Solution (mg/l)	Certified Absorbance (A)	UUC* Reading Absorbance (A)	Error (A)	Uncertainty ± (A)	k Factor	
RM-0204060810	235.0	20	0.2422	0.2418	-0.0004	0.0101	2.00	
		40	0.4866	0.4852	-0.0014	0.0115	2.00	
		60	0.7414	0.7389	-0.0025	0.0067	2.00	
		80	0.9858	0.9842	-0.0016	0.0093	2.00	
		100	1.2442	1.2414	-0.0028	0.0086	2.00	

UUC\* = Unit Under Calibration

Condition of this result of calibration : Spectrophotometer PERKINELMER Model Lambda 25 S/N 501S14123010

Resolution of Wavelength Mode 0.1 nm

Resolution of Photometric Mode 0.0001 A

Parameter Setting

Measurement Mode Wavelength, Absorbance

Wavelength Scan 1100 nm-190 nm

Scanning Speed 7.5 nm/min

Data Pitch 0.1 nm

Band width(Wavelength) 1.0 nm

Band width(Vis) 1.0 nm

Band width(Uv) 1.0 nm

Stray Light\*\* UUC\* Reading at 220 nm

Transmission T(%)	Absorbance(A)
0.0117	3.8659

\*\*Specific Acceptance :

Transmission  $\leq$  1.0 T(%), Absorbance  $\geq$  2.0 A

\*\*Stray light not TISI Accredited

The reported uncertainty is based on a standard uncertainty multiplied by a coverage factor  $k$ , providing a level of confidence of approximately 95%

End of Calibration Certificate

*T. Ketch*



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด  
S.P.S. CONSULTING SERVICE CO., LTD.  
7 ซอยพลโยธิน 24 ถนนพลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900  
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900  
Tel : (662) 939-4370-72 Fax : (662) 513-4221 E-mail : sale@spscon.com, www.spscon.com

Personal Pump Calibration Report

Calibration Method : Dry Cal Primary Flowmeter

Model : Defender 510-H

S/N : 136164

Environmental Conditions

Temperature : 25  $\pm$  3  $^{\circ}$ C  
Pressure : 1010  $\pm$  15 mmbar

Personal Pump Data				Calibration Data								
No.	Brand	Model	Serial No.	Date	Flow Rate (ml/min)						Value From Calibration Curve	
					Setting			Actual (Q std.)				
					1	2	3	1	2	3	y	R <sup>2</sup>
B41	SKC	224-PCXR4	612669	03/04/2025	1,000	1,500	2,000	1,005	1,502	2,004	1.005x - 8.923	1.000
B42	SKC	224-PCXR4	626041	03/04/2025	1,000	1,500	2,000	1,004	1,501	2,008	1.009x - 13.856	1.000
B43	SKC	224-PCXR4	034636	01/04/2025	1,000	1,500	2,000	1,012	1,497	1,996	0.990x + 15.132	1.000
B44	SKC	224-PCXR8	529341	01/04/2025	1,000	1,500	2,000	1,011	1,511	2,008	1.002x - 0.860	0.999
B45	SKC	224-PCXR8	529594	04/04/2025	1,000	1,500	2,000	993	1,512	2,003	1.009x - 14.476	1.000
B46	SKC	224-PCXR8	566743	04/04/2025	1,000	1,500	2,000	1,008	1,508	2,008	1.000x - 0.100	0.999
B47	SKC	224-PCXR8	566747	04/04/2025	1,000	1,500	2,000	999	1,510	2,010	1.010x - 14.444	1.000
B48	SKC	224-PCXR8	566753	01/04/2025	1,000	1,500	2,000	1,010	1,506	2,006	0.999x + 2.782	1.000
B49	SKC	224-PCXR8	566780	04/04/2025	1,000	1,500	2,000	1,003	1,504	2,004	1.003x - 2.183	1.000
B50	SKC	224-PCXR8	500400	04/04/2025	1,000	1,500	2,000	1,002	1,493	1,995	0.994x + 5.841	1.000
B51	SKC	224-PCXR8	500363	04/04/2025	1,000	1,500	2,000	998	1,511	2,011	1.013x - 19.465	0.999
B52	SKC	224-PCXR8	093186	02/04/2025	1,000	1,500	2,000	997	1,505	2,006	1.008x - 12.641	1.000
B53	SKC	224-PCXR8	707670	02/04/2025	1,000	1,500	2,000	1,004	1,503	2,007	1.007x - 7.992	1.000
B54	SKC	224-PCXR3	509821	02/04/2025	1,000	1,500	2,000	1,005	1,504	2,008	1.010x - 15.060	0.999
B55	SKC	224-PCXR3	510710	02/04/2025	1,000	1,500	2,000	1,001	1,495	1,997	0.996x + 5.073	1.000
B56	SKC	224-PCXR3	511450	02/04/2025	1,000	1,500	2,000	1,005	1,494	1,996	0.991x - 13.385	1.000
B57	SKC	224-PCXR3	510798	03/04/2025	1,000	1,500	2,000	997	1,511	2,009	1.014x - 21.540	0.999
B58	SKC	224-PCXR3	509852	03/04/2025	1,000	1,500	2,000	1,006	1,493	2,002	1.001x - 4.094	1.000
B59	SKC	224-PCXR3	509862	03/04/2025	1,000	1,500	2,000	995	1,502	2,003	1.012x - 21.564	1.000
B60	SKC	224-PCXR3	512655	03/04/2025	1,000	1,500	2,000	998	1,507	2,004	1.010x - 18.510	0.999
B61	SKC	224-PCXR3	503915	03/04/2025	1,000	1,500	2,000	997	1,499	2,001	1.002x - 4.374	1.000
B62	SKC	224-PCXR3	505975	01/04/2025	1,000	1,500	2,000	1,002	1,503	2,005	1.008x - 11.138	1.000
B63	SKC	224-PCXR3	511432	04/04/2025	1,000	1,500	2,000	998	1,502	1,996	0.996x + 3.970	1.000
B64	SKC	224-PCXR3	508302	04/04/2025	1,000	1,500	2,000	1,005	1,509	2,008	1.009x - 10.402	1.000
B65	SKC	224-PCXR3	508310	04/04/2025	1,000	1,500	2,000	1,004	1,503	2,007	1.010x - 14.088	1.000
B66	SKC	224-PCXR3	509861	04/04/2025	1,000	1,500	2,000	1,003	1,504	2,010	1.008x - 12.369	1.000
B67	SKC	224-PCXR3	506295	04/04/2025	1,000	1,500	2,000	1,002	1,498	2,004	0.998x + 4.290	1.000
B68	SKC	224-PCXR3	505872	04/04/2025	1,000	1,500	2,000	999	1,504	1,998	1.000x + 0.436	1.000
B69	SKC	224-PCXR3	508375	02/04/2025	1,000	1,500	2,000	1,004	1,498	2,002	0.996x + 5.501	1.000
B70	SKC	224-PCXR3	510623	02/04/2025	1,000	1,500	2,000	996	1,497	2,005	1.005x - 8.735	1.000
B71	SKC	224-PCXR3	508367	02/04/2025	1,000	1,500	2,000	1,013	1,505	2,009	1.000x + 3.294	0.999
B72	SKC	224-PCXR3	505977	02/04/2025	1,000	1,500	2,000	997	1,494	2,003	1.006x - 11.350	1.000
B73	SKC	224-PCXR3	512606	01/04/2025	1,000	1,500	2,000	1,010	1,507	2,004	0.998x + 5.129	1.000
B74	SKC	224-PCXR3	505993	01/04/2025	1,000	1,500	2,000	998	1,499	2,010	1.009x - 11.942	1.000
B75	SKC	224-PCXR3	509820	01/04/2025	1,000	1,500	2,000	995	1,511	2,004	1.011x - 18.966	0.999
B76	SKC	224-PCXR3	509811	01/04/2025	1,000	1,500	2,000	998	1,504	2,010	1.012x - 20.993	0.999
B77	SKC	224-PCXR3	508301	03/04/2025	1,000	1,500	2,000	1,007	1,509	2,008	1.001x + 3.750	1.000
B78	SKC	224-PCXR3	510677	04/04/2025	1,000	1,500	2,000	998	1,508	2,001	1.003x - 3.278	1.000
B79	SKC	224-PCXR3	510920	04/04/2025	1,000	1,500	2,000	1,001	1,501	1,994	0.999x - 1.819	1.000

Calibrated by :

Adul Dangklom  
(Mr. Adul Dangklom)

Approved by :

(Mr. Peera Detudorn)





บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด  
S.P.S. CONSULTING SERVICE CO., LTD.  
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900  
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900  
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

### Personal Pump Calibration Report

Calibration Method : Dry Cal Primary Flowmeter

Model : Defender 510-H

S/N : 136833

#### Environmental Conditions

Temperature : 25 ± 3 °C  
Pressure : 1010 ± 15 mmbar

Personal Pump Data				Calibration Data								
No.	Brand	Model	Serial No.	Date	Flow Rate (ml/min)						Value From Calibration Curve	
					Setting			Actual (Q std.)				
					1	2	3	1	2	3	y	R <sup>2</sup>
R01	SKC	224-PCXR4	602467	02/04/2025	1,000	1,500	2,000	1,003	1,506	2,001	1.003x - 1.855	1.000
R02	SKC	224-PCXR4	626450	02/04/2025	1,000	2,000	3,000	994	1,501	2,002	1.006x - 11.866	1.000
R03	SKC	224-PCXR4	691592	01/04/2025	1,000	1,500	2,000	995	1,509	2,007	1.013x - 22.400	0.999
R04	SKC	224-PCXR4	691672	02/04/2025	1,000	1,500	2,000	996	1,502	1,996	0.999x + 0.668	1.000
R05	SKC	224-PCXR4	798470	04/04/2025	1,000	1,500	2,000	995	1,511	2,005	1.010x - 16.711	0.999
R06	SKC	224-PCXR4	798456	04/04/2025	1,000	1,500	2,000	1,002	1,499	2,003	1.004x - 5.745	1.000
R07	SKC	224-PCXR4	798480	04/04/2025	1,000	1,500	2,000	1,005	1,504	2,007	1.011x - 16.099	0.999
R08	SKC	224-PCXR4	883215	04/04/2025	1,000	1,500	2,000	1,002	1,503	2,004	1.014x - 23.623	0.999
R09	SKC	224-PCXR4	034650	02/04/2025	1,000	1,500	2,000	999	1,497	2,011	1.009x - 11.282	1.000
R10	SKC	224-PCXR4	091765	01/04/2025	1,000	1,500	2,000	1,002	1,505	2,003	1.012x - 20.705	0.999
R11	SKC	224-PCXR4	091763	02/04/2025	1,000	1,500	2,000	997	1,504	2,005	1.005x - 4.550	1.000
R12	SKC	224-PCXR4	091568	02/04/2025	1,000	1,500	2,000	998	1,513	2,004	1.015x - 25.798	0.999
R13	SKC	224-PCXR4	091638	03/04/2025	1,000	1,500	2,000	996	1,502	1,999	1.003x - 5.821	1.000
R14	SKC	224-PCXR4	091764	03/04/2025	1,000	1,500	2,000	1,002	1,503	1,997	0.997x + 5.785	1.000
R15	SKC	224-PCXR8	529457	01/04/2025	1,000	1,500	2,000	996	1,501	2,001	1.002x - 5.453	1.000
R16	SKC	224-PCXR8	529643	02/04/2025	1,000	1,500	2,000	999	1,506	1,998	0.998x + 4.829	1.000
R17	SKC	224-PCXR8	529645	02/04/2025	1,000	1,500	2,000	993	1,504	2,004	1.009x - 19.210	1.000
R18	SKC	224-PCXR8	566756	04/04/2025	1,000	1,500	2,000	1,005	1,503	2,008	1.007x - 9.639	1.000
R19	SKC	224-PCXR8	566802	04/04/2025	1,000	1,500	2,000	996	1,495	1,997	1.000x - 2.051	1.000
R20	SKC	224-PCXR8	529089	02/04/2025	1,000	1,500	2,000	999	1,498	1,999	1.004x - 12.497	1.000
R21	SKC	224-PCXR8	665728	02/04/2025	1,000	1,500	2,000	994	1,502	1,996	1.000x - 2.818	1.000
R22	SKC	224-PCXR8	707444	03/04/2025	1,000	1,500	2,000	999	1,507	2,004	1.009x - 16.603	0.999
R23	SKC	224-PCXR8	761067	03/04/2025	1,000	1,500	2,000	997	1,496	1,997	1.001x - 3.342	1.000
R24	SKC	224-PCXR8	707893	02/04/2025	1,000	1,500	2,000	1,005	1,504	2,012	1.008x - 11.430	0.999
R25	SKC	224-PCXR8	761052	01/04/2025	1,000	1,500	2,000	1,002	1,493	2,010	1.006x - 8.771	1.000
R26	SKC	224-PCXR8	707956	02/04/2025	1,000	1,500	2,000	997	1,504	1,997	1.001x - 2.663	1.000
R27	SKC	224-PCXR8	707398	02/04/2025	1,000	1,500	2,000	996	1,495	2,001	1.007x - 19.305	0.999
R28	SKC	224-PCXR8	707481	03/04/2025	1,000	1,500	2,000	1,013	1,507	2,004	0.996x + 9.887	1.000
R29	SKC	224-PCXR8	707402	04/04/2025	1,000	1,500	2,000	998	1,499	2,010	1.010x - 19.297	1.000
R30	SKC	224-PCXR8	093811	02/04/2025	1,000	1,500	2,000	1,008	1,505	2,008	1.006x - 6.261	1.000
R31	SKC	224-PCXR8	093183	02/04/2025	1,000	1,500	2,000	1,002	1,501	1,994	0.998x - 0.140	1.000
R32	SKC	224-PCXR8	671950	01/04/2025	1,000	1,500	2,000	1,001	1,498	1,997	0.997x + 3.786	1.000
R33	SKC	224-PCXR4	626254	01/04/2025	1,000	1,500	2,000	1,006	1,497	2,001	0.995x + 7.736	1.000
R34	SKC	224-PCXR4	626131	01/04/2025	1,000	1,500	2,000	994	1,506	2,006	1.009x - 17.998	1.000
R35	SKC	224-PCXR8	707460	01/04/2025	1,000	1,500	2,000	1,006	1,505	2,014	1.010x - 14.668	0.999
R36	SKC	224-PCXR8	707446	04/04/2025	1,000	1,500	2,000	998	1,500	1,995	1.000x - 2.067	1.000
R37	SKC	224-PCXR8	707432	02/04/2025	1,000	1,500	2,000	1,005	1,494	2,006	0.998x + 4.721	1.000
R38	SKC	224-PCXR8	707349	03/04/2025	1,000	1,500	2,000	996	1,511	2,007	1.012x - 19.485	0.999
R39	SKC	224-PCXR8	761095	02/04/2025	1,000	1,500	2,000	1,005	1,505	2,008	1.004x - 4.026	1.000

Calibrated by :

Adul Dangklom  
(Mr. Adul Dangklom)

Approved by :

(Mr. Feera Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด  
S.P.S. CONSULTING SERVICE CO., LTD.  
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900  
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900  
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

Personal Pump Calibration Report

Calibration Method : Dry Cal Primary Flowmeter

Model : Defender 510-H

S/N : 136833

Environmental Conditions

Temperature : 25  $\pm$  3  $^{\circ}$ C  
Pressure : 1010  $\pm$  15 mmbar

Personal Pump Data				Calibration Data								
No.	Brand	Model	Serial No.	Date	Flow Rate (mL/min)						Value From Calibration Curve	
					Setting			Actual (Q std.)				
					1	2	3	1	2	3	y	R <sup>2</sup>
R40	SKC	224-PCXR4	612753	03/04/2025	1,000	1,500	2,000	1,013	1,505	2,008	0.996x + 6.748	0.999
R41	SKC	224-PCXR4	626140	01/04/2025	1,000	1,500	2,000	1,006	1,506	2,009	1.005x - 6.157	1.000
R42	SKC	224-PCXR4	626463	02/04/2025	1,000	1,500	2,000	1,005	1,495	2,002	0.997x + 5.089	1.000
R43	SKC	224-PCXR4	626129	04/04/2025	1,000	1,500	2,000	1,004	1,504	2,008	1.011x - 15.436	1.000
R44	SKC	224-PCXR4	602753	02/04/2025	1,000	1,500	2,000	999	1,492	2,001	1.004x - 13.988	0.999
R45	SKC	224-PCXR4	626137	03/04/2025	1,000	1,500	2,000	1,001	1,501	1,996	0.994x + 9.247	1.000

Calibrated by :

Adul Dangklom  
(Mr. Adul Dangklom)

Approved by :

Peera Detudom  
(Mr. Peera Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด  
**S.P.S. CONSULTING SERVICE CO., LTD.**  
 7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900  
 7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900  
 Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

Rotameter Calibration Report (For Personal Pump High Flow Adjust)

Calibration Method : Dry Cal Primary Flowmeter

Model : Defender 510-H

S/N : 136164

Calibration Data

Rotameter Data			Calibration Data								
No.	Brand	Model	Date	Flow Rate (mL/min)						Value From Calibration Curve	
				Flow Rate (Reading)			Actual (Q std.)				
				1	2	3	1	2	3	y	R <sup>2</sup>
H-R01	Dwyer	VFB-65	02/04/2025	500	1,000	2,000	499.6	998.8	2004.8	1.001x - 3.678	1.000
H-R02	Dwyer	VFB-65	02/04/2025	500	1,000	2,000	501.7	997.1	1991.5	0.998x + 0.386	0.999
H-R03	Dwyer	VFB-65	01/04/2025	500	1,000	2,000	499.8	999.7	1992.8	1.000x + 1.316	1.000
H-R04	Dwyer	VFB-65	04/04/2025	500	1,000	2,000	500.2	999.4	1989.2	0.999x + 1.870	0.999
H-R05	Dwyer	VFB-65	04/04/2025	500	1,000	2,000	499.9	1000.8	1994.5	1.000x + 0.815	1.000
H-R06	Dwyer	VFB-65	03/04/2025	500	1,000	2,000	500.5	1001.3	1990.7	0.997x + 4.894	0.999

Calibrated by :

Adul Dangklom  
 (Mr.Adul Dangklom)

Approved by :

(Mr. Peera Detudom)





บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด

S.P.S. CONSULTING SERVICE CO., LTD.

7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900  
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900  
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

Calibration Report					
Non-Dispersive Infrared CO Analyzer					
Date :	05 May 2025	Brand :	API	Model :	300E
No.	CO-R02			Serial No.	171-S
Calibrator (Dilution System)					
Brand : Teledyne			Model : 700E		
Last Cal. Date : 28 October 2024			Serial No. : 201-S		
Reference Standard Gas					
Standard Gas : Carbon Monoxide (CO)			Cylinder No. : D711839		
Certified Date : 14 March 2024		Expired Date : 14 March 2032		Cylinder Conc. : 4,580 ppm	
Calibrating Condition					
Pressure : 1011 mmbar		Temp. : 24.6 °C		% RH : 50	
Calibration Setting					
Span	Initial Reading (Before Adj.), PPM			Final Reading (After Adj.), PPM	
Set Point	Expected Concentration	Analyzer Response	%Dif	Analyzer Response	
Zero	0	0.11	-	0	
CO Span	40.00	40.10	0.250	40.00	
API Model 300E CO Analyzer Check List					
Parameter	Observed Value	Units	Nominal Range		
Range	50	PPM	0-1000 ppm		
Stability	0.10	PPM	< 1 ppm With Zero Air		
CO Measure	4014.7	mV	2500-4800 mV		
CO Reference	3948.1	mV	2500-4800 mV		
Measure/Reference Ratio	1.180	-	1.1-1.3 W/Zero Air		
Sample Pressure	28.7	In-Hg-A	~2" < Ambient Absolute Pressure		
Sample Flow	804	CC/Min	800 ± 10%		
Sample Temperature	48.2	°C	48 ± 4		
Bench Temperature	48.0	°C	48 ± 2		
Wheel Temperature	68.2	°C	68 ± 2		
Box Temperature	30.8	°C	Ambient Temp + 7 ± 10		
Photo-Drive	3038.5	mV	250 mV to 4750 mV		
Slope	1.017	-	1.0 ± 0.3		
Offset	0.2	-	0 ± 0.3		

Calibrated by :

Adul Dangklom

(Mr. Adul Dangklom)

Approved by :

(Mr. Peera Detudom)



## MAINTENANCE AND TEST CERTIFICATE MODEL

### OPTIMA 5300DV

<b>Customer :</b> <u>S.P.S.Consulting Service Co.,Ltd</u>	Date Tested: <u>January 6, 2025</u>	
	Recommendation Recertification	
<b>Address :</b> <u>7 Soi Phaholyothin 24</u>	Period <u>6</u> Months	
<u>Paholyothin Road</u>	Recertification Due: <u>July 6, 2025</u>	
<u>Jompol Chatuchak, Bangkok 1090</u>	Date Last Certified: <u>July 4, 2024</u>	
<b>User Name:</b> <u>K.Phenpha Viphasthawat</u>	Visit Number: <u>2 of 2</u>	
<b>Phone:</b> <u>083-9269252</u>	PerkinElmer Phone: <u>02-719-6420 ext 206</u>	
<b>Fax:</b> <u>02-513-4221</u>	PerkinElmer Fax: <u>02-318-5597</u>	

CONFIGURATION TESTED		ACCESSORIES/COMPONENT NOT INCLUDED
<b>MODEL</b>	<b>SERIAL NUMBER</b>	
<u>OPTIMA 5300DV</u>	<u>077C7042401</u>	
<b>TESTED EQUIPMENT</b>	<b>CALIBRATION NUMBER</b>	<b>EXPIRATION</b>
<u>IPV Methods</u>		
<b>TEST STANDARD USED</b>	<b>PART NUMBER</b>	<b>EXPIRATION DATE</b>
<u>Multielement Standard</u>	<u>N069-1579</u>	<u>December 30, 2025</u>
<u>Wavecal Solution</u>	<u>N058-2152</u>	<u>April 30, 2025</u>
<u>VIS Wavecal solution</u>	<u>N930-2946</u>	<u>December 30, 2025</u>
<u>Instrument Cal. STD4</u>	<u>N930-0221</u>	<u>August 30, 2025</u>
<b>CUSTOMER SUPPLIED</b>	<b>COMMENTS</b>	<b>CUSTOMER INITIALS</b>
<u>2 % HNO3</u>		
<u>10 % HNO3</u>		





## MAINTENANCE AND TEST CERTIFICATE MODEL

### OPTIMA 5300DV

**SERIAL NUMBER** 077C7042401**DATE TESTED** January 6, 2025**1. MECHANICAL CHECKS**

A. Inspect and clean all fans and filters.

☐ OK

B. Inspect and replace as necessary, all torch components including the RF coil.

☐ OK

C. Inspect all tubing for sign of clacking or leaking.

☐ OK

D. Adjust water and gas pressure regulator settings.

☐ OK

E. Inspect and leak check pneumatics drawers.

☐ OK

F. Clean the exterior of the instrument.

☐ OK**2. OPTICAL CHECKS**

A. Inspect and clean all optical components.

☐ OK

B. As required, check and replace all purgefilters.

☐ OK

C. Recheck optical alignment.

☐ OK**3. COOLING SYSTEM CHECKS**

A. Perform preventive maintenance on chiller.

☐ OK

B. Flush out the chiller every year.

☐ N/A**4. PERFORMANCE CHECKS**

A. Torch View Alignment.

☐ OK

B. Wavelength Calibration.

☐ OK



## MAINTENANCE AND TEST CERTIFICATE MODEL

### OPTIMA 5300DV

SERIAL NUMBER : 077C7042401DATE TESTED : January 6, 2025

PARAMETER		SPECIFICATION		FINAL VALUE	
Spectral Resolution : UV	As 193.696 nm	≤ 0.007		0.00519	
	Ni 231.604 nm	≤ 0.008		0.00667	
	Ni 341.476 nm	≤ 0.012		0.00757	
Spectral Resolution : VIS	La 408.672 nm	≤ 0.020		0.01621	
	Ba 455.403 nm	≤ 0.025		0.02183	
Precision					
	As 193.656 nm	% RSD	< 1.0	0.51	%
	Zn 213.856 nm	% RSD	< 1.0	0.48	%
	Mn 257.610 nm	% RSD	< 1.0	0.03	%
	La 379.478 nm	% RSD	< 1.0	0.05	%
	Ba 455.403 nm	% RSD	< 1.0	0.07	%
	Ba 493.408 nm	% RSD	< 1.0	0.04	%
Detection Limits : Axial	Tl 190.080 nm	3(sd)		10.65	ppb
	As 193.696 nm	3(sd)		2.48	ppb
	Pb 220.353 nm	3(sd)		3.09	ppb
Detection Limits : Radial	As 193.696 nm	3(sd)		12.41	ppb
	Zn 213.856 nm	3(sd)		0.91	ppb
	Mn 257.610 nm	3(sd)		0.13	ppb
	La 379.478 nm	3(sd)		4.74	ppb
	Ba 455.403 nm	3(sd)		0.10	ppb
	Ba 493.408 nm	3(sd)		0.18	ppb
BEC : Axial (IB X 500)/(IS-IB)	Cd 226.502 nm	≤ 150 ppb		14.22	
BEC : Radial (IB X 1000)/(IS-IB)	Mn 257.610 nm	≤ 45 ppb		6.14	



## MAINTENANCE AND TEST CERTIFICATE MODEL

### OPTIMA 5300DV

SERIAL NUMBER 077C7042401DATE TESTED January 6, 2025**Remarks :**

Commissioning follow as commissioning performance sheets.

---

---

---

---

---

---

---

---

This is to certify that the above tests have been performed and the configuration tested



meets



does not meet

the PerkinElmer Specifications listed on this certificate.

This certificate does not modify PerkinElmer's standard terms and condition of sale,  
including warranty terms.

**Service Department PerkinElmer Ltd.****Authorized Representative:**

( Wiphan Promlumda )

Service Engineer

## MAINTENANCE REPORT AND CALIBRATION CERTIFICATE

### ATOMIC ABSORPTION SPECTROPHOTOMETER MODEL

PinAAcle 900T

<b>Customer :</b>	<u>S.P.S.Consulting Service Co.,Ltd</u>	<b>Date Tested:</b>	<u>January 6, 2025</u>
<b>Address :</b>	<u>7 Soi Phaholyothin 24</u>	<b>Recommendation Recertification</b>	
	<u>Paholyothin Road</u>	<b>Period</b>	<u>6</u> Months
	<u>Jompol Chatuchak, Bangkok 10900</u>	<b>Recertification Due:</b>	<u>July 6, 2025</u>
<b>User Name:</b>	<u>K.Phenpha Vipasthawatt</u>	<b>Date Last Certified:</b>	<u>July 4, 2024</u>
<b>Phone:</b>	<u>083-9269252</u>	<b>Visit Number:</b>	<u>1 OF 2</u>
<b>Email:</b>	<u></u>	<b>PerkinElmer Phone:</b>	<u>02-719-6420 ext 204</u>
		<b>PerkinElmer Fax:</b>	<u>02-318-5597</u>

CONFIGURATION TESTED		
MODEL	SERIAL NUMBER	SOFTWARE
<u>PinAAcle 900T</u>	<u>PTCS14111103</u>	<u>Wiblab V5.1</u>
<u>AS 900</u>	<u></u>	<u></u>
<u></u>	<u></u>	<u></u>
<u></u>	<u></u>	<u></u>
<u></u>	<u></u>	<u></u>
TEST STANDARD USED	PART NUMBER	EXPIRATION DATE
<u>Copper</u>	<u>N9300183</u>	<u>APR 30 2025</u>
<u>GFAAS Mixed standard</u>	<u>N9300244</u>	<u>FEB 28 2025</u>
<u>MG0-042</u>	<u>N101-3000</u>	<u></u>
<u>MG2-045</u>	<u>N101-3002</u>	<u></u>
<u></u>	<u></u>	<u></u>



# MAINTENANCE REPORT AND CALIBRATION CERTIFICATE

## ATOMIC ABSORPTION SPECTROPHOTOMETER MODEL

PinAAcle 900T

SERIAL NUMBER	PTCS14111103	DATE TESTED	January 6, 2025
<b>1. INSTRUMENT CHECKS</b>			
A. The Mirror and Lenses Condition			<input type="text" value="OK"/>
B. Grating Condition			<input type="text" value="OK"/>
C. Replace or Clean Dust Filter			<input type="text" value="OK"/>
D. Cleaning the Contact Cylinders			<input type="text" value="OK"/>
E. Cleaning the Furnace Windows			<input type="text" value="OK"/>
F. Cleaning the Burner Head			<input type="text" value="OK"/>
G. Cleaning the Nebulizer			<input type="text" value="OK"/>
H. Cleaning the Drain System			<input type="text" value="OK"/>
<b>2. AUTOSAMPLE CHECK</b>			
A. Sampling and Arm			<input type="text" value="OK"/>
B. Sampling & Rinse Pump			<input type="text" value="OK"/>
C. Sample Position & Clean			<input type="text" value="OK"/>
<b>3. COOLING SYSTEM CHECKS</b>			
A. Clean and Change Distill water			<input type="text" value="OK"/>
B. Themensor			<input type="text" value="OK"/>
<b>4. FIAS CHECKS</b>			
A. Pump and 5 Port Valve			<input type="text" value="N/A"/>
B. Chemifold and Tubing			<input type="text" value="N/A"/>
C. Power Supply			<input type="text" value="N/A"/>
D. Flow meter and Gas system			<input type="text" value="N/A"/>

# MAINTENANCE REPORT AND CALIBRATION CERTIFICATE

## ATOMIC ABSORPTION SPECTROPHOTOMETER MODEL

**PinAAcle 900T**

<b>SERIAL NUMBER</b>	<u>PTCS14111103</u>	<b>DATE TESTED</b>	<u>January 6, 2025</u>
<b>PARAMETER</b>		<b>SPECIFICATION</b>	<b>ACTUAL VAULE</b>
<b>A. Flame Mode Tests</b>			
1. Detector-Linearity with Barium (553.55 nm)			
Neutral Density Filter 0.2 :	<u>0.2042</u>	Abs. $\pm$ 5%	<u>0.2029</u> Abs.
Neutral Density Filter 1.0 :	<u>0.9798</u>	Abs. $\pm$ 5%	<u>1.0137</u> Abs.
2. Baseline Noise at 1 Abs with Barium (553.55 nm)			
(at an integration time of 0.5 seconds			
and 99 replicates)			
		SD $\leq$ 0.010 Abs.	<u>0.0016</u> Abs.
3. AA Baseline with Copper (Cu 324.75 nm)			
(at an integration time of 0.5 seconds			
and 99 replicates)			
		SD $\leq$ 0.001 Abs.	<u>0.0002</u> Abs.
4. D <sub>2</sub> Background Compensation (Copper 324.75 nm)			
with Neutral Density Filter 1.0		Absorbance $\leq$ 0.010 Abs	<u>0.0020</u> Abs.
5. AA-BG Baseline Noise with Copper (324.75 nm)			
(at an integration time of 2.0 seconds			
and 99 replicates)			
		SD $\leq$ 0.005 Abs.	<u>0.0002</u> Abs.
6. AA-BG Baseline Noise with Arsenic (193.70 nm)			
(at an integration time of 2.0 seconds			
and 99 replicates)			
		SD $\leq$ 0.005 Abs.	<u>0.0007</u> Abs.

## MAINTENANCE REPORT AND CALIBRATION CERTIFICATE

### ATOMIC ABSORPTION SPECTROPHOTOMETER MODEL

PinAAcle 900T

<b>SERIAL NUMBER</b>	<u>PTCS14111103</u>	<b>DATE TESTED</b>	<u>January 6, 2025</u>
<b>PARAMETER</b>	<b>SPECIFICATION</b>	<b>ACTUAL VAULE</b>	
7. Flame Interlock Shutdown	Shutdown correct?	<div>OK</div>	
8. Flame Sensitivity with Copper (324.75 nm)			
(5 mg/L Cu Standard a read time of 10 seconds			
10 replicates, standard burner and Stainless stell nebulizer)			
	Sensitivity $\geq 0.250$ Abs.	<u>0.3115</u>	Abs.
(2 mg/L Cu Standard a read time of 10 seconds			
10 replicates, standard burner and High sensitivity nebulizer)			
	Sensitivity $\geq 0.250$ Abs.	<u>N/A</u>	Abs.

## MAINTENANCE REPORT AND CALIBRATION CERTIFICATE

### ATOMIC ABSORPTION SPECTROPHOTOMETER MODEL

PinAAcle 900T

SERIAL NUMBER	PTCS14111103	DATE TESTED	January 6, 2025
PARAMETER	SPECIFICATION	ACTUAL VAULE	
B. THGA Tests			
1. Furnace Gas Flows			
Internal Flow	250 ± 25 mL/min	250	mL/min
External Flow	100 ± 10 mL/min	100	mL/min
2. Chromium Baseline Noise (357.87 nm)			
(mesure 5 furnace dry firings without any sample)			
	Baseline ≤ 0.005 Int.Abs	0.0012	
	SD ≤ 0.005 Int.Abs	0.0002	Int.Abs.
3. Chromium Characteristic Mass(m <sub>0</sub> ) and Precition (357.87 nm)			
(measure 5 furnace firing using 20 ul			
sample injections of 10 ug/L Cr standard)			
	m0 Results ≤ 7.0 pg/0.0044A-s	5.4	pg/0.0044A-s
	Precision ≤ 2.0%	1.15	%
4. Copper Characteristic Mass(m <sub>0</sub> ) and Zeeman Ratio (324.75 nm)			
(measure 5 furnace firing using 20 ul			
sample injections of 25 ug/L Cu standard)			
	m0 Results ≤ 16.5 pg/0.0044A-s	14.4	pg/0.0044A-s
	Zeeman Ratio 0.52 + 0.04	0.542	



## MAINTENANCE REPORT AND CALIBRATION CERTIFICATE

### ATOMIC ABSORPTION SPECTROPHOTOMETER MODEL

**PinAAcle 900T**

**SERIAL NUMBER** PTCS14111103 **DATE TESTED** January 6, 2025

Remarks :

- Neutral Density Filter refer to data sheet

- Zeeman Ratio =  $\frac{\text{Atomic Signal(peak area)}}{\text{Atomic Signal(peak area)+Background Signal(peak area)}}$

= 0.1635/0.1635+0.1378

0.542

This is to certify that the above tests have been performed and the configuration tested



meets




does not meet

the PerkinElmer Specifications listed on this certificate.

This certificate does not modify PerkinElmer's standard terms and condition of sale, including warranty terms.

**Service Department PerkinElmer Ltd.**

Customer Service Engineer:



( Wiphan Promlumda )

Service Engineer

ลำดับที่ 3

คุณภาพน้ำ

**QUALITY CALIBRATION CO., LTD.**

235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160

Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584



CERTIFICATE No : 24E6416

REFERENCE No : 73694-1

PAGE : 1 OF 3

**Certificate of Calibration**

**EQUIPMENT** : pH METER

**MANUFACTURER** : HANNA

**MODEL** : HI 3512

**SERIAL No** : TH118035

**ID No** : pH 04/56

**CONDITION AS RECEIVED** : USED ITEM

**SUBMITTED BY** : S.P.S. CONSULTING SERVICE CO., LTD.  
7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN RD.,  
JOMPOL, CHATUCHAK, BANGKOK 10900

**CALIBRATED BY** : ATSAWIN Y.

**CALIBRATION DATE** : 27-Jun-24

**APPROVED BY** :   
PONGSAK J.

**ISSUED DATE** : 27-Jun-24

**RECEIVED DATE** : 24-Jun-24

THIS CERTIFICATE MAY NOT BE REPRODUCED OTHER THAN IN FULL EXCEPT WITH THE PRIOR WRITTEN APPROVAL OF  
QUALITY CALIBRATION CO., LTD.



**QUALITY CALIBRATION CO., LTD.**

235 Petchkasem 63/2 Road, Laksong, Bangkac, Bangkok 10160

Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

CERTIFICATE No : 24E6416

PAGE : 2 OF 3

**Calibration Report**

EQUIPMENT : pH METER  
MANUFACTURER : HANNA  
ID No : pH 04/56  
RECEIVED DATE : 24-Jun-24  
AMBIENT TEMPERATURE : 23 ° C ± 3 ° C

MODEL : HI 3512  
SERIAL NUMBER : TH118035  
CALIBRATION DATE : 27-Jun-24  
RELATIVE HUMIDITY : 50 % RH ± 10% RH

**CONDITION OF THIS RESULTS OF CALIBRATION**

1. THIS INSTRUMENT WAS CALIBRATED BY DIRECT MEASUREMENT METHOD BASED ON WI-TQ-062 AND WI-TQ-063. THE DISPLAY UNIT WAS TESTED BY GENERATING STANDARD VOLTAGE TO THE UNIT AND READING THE VALUE COMPARED WITH THE CALCULATED VALUE. THE DISPLAY AND ELECTROD WAS CALIBRATED BY USING STANDARD pH BUFFER
2. REFERENCE STANDARD INSTRUMENTS :-

<u>INSTRUMENT</u>	<u>MODEL</u>	<u>SERIAL No/ LOT No</u>	<u>CERTIFICATE No</u>	<u>DUE DATE</u>
1) pH STANDARD SOLUTION	00651-06	CC784945	4880-14413915	24-Aug-25
2) pH STANDARD SOLUTION	00651-08	CC785578	4881-14430633	31-Aug-25
3) pH STANDARD SOLUTION	00651-10	CC787086	4882-14483317	21-Sep-25
4) PROCESS CALIBRATOR	CA150	91S6079	24E1251	09-Apr-25
5) BATH	260014	1247 48074	23T9014	13-Sep-24
6) THERMOMETER WITH PROBE	421504	55000379	23T9623	13-Sep-24

3. THE CERTIFICATE IS VALID FOR THE ITEM CALIBRATED AS SHOWN ON THE DATE AND PLACE OF CALIBRATION ONLY.
4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.
5. THIS CERTIFICATE IS TRACEABLE TO SI UNIT MAINTAINED AT :-
  - NATIONAL INSTITUTE OF STANDARD AND TECHNOLOGY, USA.
  - NATIONAL INSTUTITE OF METROLOGY (THAILAND)

**RESULT OF CALIBRATION : ADJUSTMENT****1. DISPLAY UNIT ONLY**SLOPE FACTOR  $k = 2.303 RT/F = 59 \text{ mV/pH}$ 

mV APPLIED	UUC READING (mV)	CORRECTION (mV)	UUC READING (pH)	UNCERTAINTY OF MEASUREMENT (± mV)	COVERAGE FACTOR k
414.11	414.8	-0.69	-0.115	0.15	2.00
354.95	355.5	-0.55	0.884	0.15	2.00
295.80	296.4	-0.60	1.885	0.15	2.00
236.64	237.1	-0.46	2.886	0.15	2.00
177.48	178.0	-0.52	3.887	0.15	2.00
118.32	118.8	-0.48	4.887	0.15	2.00
59.16	59.6	-0.44	5.887	0.15	2.00
0.00	0.4	-0.40	6.888	0.15	2.00
-59.16	-58.7	-0.46	8.101	0.15	2.00
-118.32	-117.9	-0.42	9.345	0.15	2.00
-177.48	-177.4	-0.08	10.589	0.15	2.00
-236.64	-236.4	-0.24	11.834	0.15	2.00
-295.80	-294.5	-1.30	13.077	0.15	2.00
-354.95	-354.7	-0.25	14.322	0.15	2.00
-414.11	-413.9	-0.21	15.565	0.15	2.00

END OF CALIBRATION REPORT PAGE 2 OF 3





# QUALITY CALIBRATION CO., LTD.

235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160

Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

CERTIFICATE No : 24E6416

PAGE : 3 OF 3

## Calibration Report

### RESULT OF CALIBRATION (CONTINUE) :

#### 2. DISPLAY UNIT WITH pH ELECTRODE S/N: 09081C6M

STANDARD pH BUFFER SOLUTION (pH)	UUC READING (pH)	CORRECTION (pH)	VALUE BEFORE ADJUSTMENT	UNCERTAINTY OF MEASUREMENT (± pH)	COVERAGE FACTOR k
4.015	4.011	0.004	3.905	0.012	2.00
7.003	7.003	0.000	6.972	0.012	2.00
10.009	10.014	-0.005	9.570	0.014	2.00

#### 3. DISPLAY UNIT WITH TEMPERATURE

STANDARD READING (°C)	UUC READING (°C)	CORRECTION (°C)	VALUE BEFORE ADJUSTMENT	UNCERTAINTY OF MEASUREMENT (± °C)	COVERAGE FACTOR k
25.004	25.0	0.004	---	0.0085	2.00

#### 4. PERCENT SLOPE 100%

UUC : UNIT UNDER CALIBRATION

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR k, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT





CERTIFICATE No : 24M2229

REFERENCE No : 72448-3

PAGE : 1 OF 2

**Certificate of Calibration**

**EQUIPMENT** : DIGITAL BALANCE

**MANUFACTURER** : SARTORIUS

**MODEL** : BSA224S-CW

**SERIAL No** : 36591843

**ID No** : BA 09/61

**CONDITION AS RECEIVED** : USED ITEM

**SUBMITTED BY** : S.P.S. CONSULTING SERVICE CO., LTD.  
7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN RD.,  
JOMPOL, CHATUCHAK, BANGKOK 10900

**CALIBRATED BY** : ATSAWIN Y.

**CALIBRATION DATE** : 08-Mar-24

**APPROVED BY** :  PONGSAK J.

**ISSUED DATE** : 14-Mar-24

**RECEIVED DATE** : 08-Mar-24





CERTIFICATE No : 24M2229

PAGE : 2 OF 2

## Calibration Report

**EQUIPMENT** : DIGITAL BALANCE **MODEL** : BSA224S-CW  
**MANUFACTURER** : SARTORIUS **S/N** : 36591843  
**ID No** : BA 09/61 **RECEIVED DATE** : 08-Mar-24  
**AIR PRESSURE** : 1010mbar  $\pm$  1mbar **CALIBRATION DATE** : 08-Mar-24  
**AMBIENT TEMPERATURE** : 25° C  $\pm$  1° C **RELATIVE HUMIDITY** : 55 %RH  $\pm$  10 % RH

### CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED BY ACCORDING TO UKAS LAB 14 EDITION 6:2019 BY USING KNOWN WEIGHT STANDARD WEIGHT. THE BALANCE WAS NOT ADJUSTED BEFORE CALIBRATION. THE BALANCE HAS NO ZERO TRACKING FUNCTION. REPEATABILITY WAS MEASURED BY USING 10 REPEATED MEASUREMENTS. LINEARITY WAS MEASURED COVERING 10 POINTS, EVENLY SPREAD OVER THE RANGE. THE INSTRUMENT WAS SET ZERO BEFORE PERFORMING THE LINEARITY TEST. OFF-CENTER LOADING WAS MEASURED BY USING STANDARD WEIGHTS PLACED ON THE PAN AND MOVED TO VARIOUS POSITIONS ON THE PAN.

2. REFERENCE STANDARD INSTRUMENTS :-

<u>INSTRUMENT</u>	<u>MODEL</u>	<u>SERIAL No</u>	<u>CERTIFICATE No</u>	<u>DUE DATE</u>
1) STANDARD WEIGHT SET	E2	QK-I-151	M2302013S	02-Feb-25
2) STANDARD WEIGHT	E2	15843	M2302014S	02-Feb-25

3. THE CERTIFICATE IS VALID FOR THE ITEM CALIBRATED AS SHOWN ON THE DATE AND PLACE OF CALIBRATION ONLY.

4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.

5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-

- NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH CENTRAL BUREAU OF WEIGHTS&MEASURES

### RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

1. ZERO SETTING FUNCTION : NORMAL


2. TARE FUNCTION : NORMAL

3. REPEATABILITY OF READING AT 200 g WAS 0 g

4. DEPARTURE FROM NOMINAL VALUE/ LINEARITY

NOMINAL VALUE (g)	BALANCE READING (g)	CORRECTION (g)	UNCERTAINTY ( $\pm$ g)
0.0	0.0000	0.0000	0.000082
0.1	0.1000	0.0000	0.000083
0.2	0.2000	0.0000	0.000083
0.5	0.5000	0.0000	0.000083
1.0	1.0000	0.0000	0.000084
2.0	2.0000	0.0000	0.000084
5.0	5.0000	0.0000	0.000086
10.0	10.0000	0.0000	0.000089
20.0	20.0001	-0.0001	0.000094
50.0	50.0000	0.0000	0.00012
100.0	100.0001	-0.0001	0.00019
200.0	200.0000	0.0000	0.00032

5. OFF CENTER LOADING ERROR



POINT	READING (g)
1	100.0000
2	100.0000
3	100.0000
4	100.0000
5	100.0000
OFF-CENTER LOADING	0.0000

NOTE: THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR  $k=2$ , PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT





CERTIFICATE No : 25M2256  
REFERENCE No : 76365-3

PAGE : 1 OF 2

## Certificate of Calibration

**EQUIPMENT** : DIGITAL BALANCE

**MANUFACTURER** : SARTORIUS

**MODEL** : BSA224S-CW

**SERIAL No** : 36591843

**ID No** : BA09/61

**CONDITION AS RECEIVED** : USED ITEM

**SUBMITTED BY** : S.P.S. CONSULTING SERVICE CO., LTD.  
7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN RD.,  
JOMPOL, CHATUCHAK, BANGKOK 10900

**CALIBRATED BY** : ATSAWIN Y.

**CALIBRATION DATE** : 07-Mar-25

**APPROVED BY** :   
PONGSAK J.

**ISSUED DATE** : 13-Mar-25

**RECEIVED DATE** : 07-Mar-25

THIS CERTIFICATE MAY NOT BE REPRODUCED OTHER THAN IN FULL EXCEPT WITH THE PRIOR WRITTEN APPROVAL OF  
QUALITY CALIBRATION CO., LTD.







CERTIFICATE No : 25M2256

PAGE : 2 OF 2

## Calibration Report

EQUIPMENT : DIGITAL BALANCE MODEL : BSA224S-CW  
MANUFACTURER : SARTORIUS S/N : 36591843  
ID No : BA09/61 RECEIVED DATE : 07-Mar-25  
AIR PRESSURE : 1009mbar  $\pm$  1mbar CALIBRATION DATE : 07-Mar-25  
AMBIENT TEMPERATURE : 24°C  $\pm$  1°C RELATIVE HUMIDITY : 52 %RH  $\pm$  10 % RH

### CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED BY ACCORDING TO UKAS LAB 14 EDITION 6:2019 BY USING KNOWN WEIGHT STANDARD WEIGHT. THE BALANCE WAS NOT ADJUSTED BEFORE CALIBRATION. THE BALANCE HAS NO ZERO TRACKING FUNCTION. REPEATABILITY WAS MEASURED BY USING 10 REPEATED MEASUREMENTS. LINEARITY WAS MEASURED COVERING 10 POINTS, EVENLY SPREAD OVER THE RANGE. THE INSTRUMENT WAS SET ZERO BEFORE PERFORMING THE LINEARITY TEST. OFF-CENTER LOADING WAS MEASURED BY USING STANDARD WEIGHTS PLACED ON THE PAN AND MOVED TO VARIOUS POSITIONS ON THE PAN.

### 2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) STANDARD WEIGHT SET	E2	QK-I-151	C02250116	28-Jan-27
2) STANDARD WEIGHT	E2	15843	C02250117	29-Jan-27

3. THE CERTIFICATE IS VALID FOR THE ITEM CALIBRATED AS SHOWN ON THE DATE AND PLACE OF CALIBRATION ONLY.

4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.

5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-

- NATIONAL INSTITUTE OF METROLOGY (THAILAND)

### RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

1. ZERO SETTING FUNCTION : NORMAL


2. TARE FUNCTION : NORMAL

3. REPEATABILITY OF READING AT 200 g WAS 0.000071 g

4. DEPARTURE FROM NOMINAL VALUE/ LINEARITY

NOMINAL VALUE (g)	BALANCE READING (g)	CORRECTION (g)	UNCERTAINTY ( $\pm$ g)
0.00	0.0000	0.0000	0.00012
0.10	0.1000	0.0000	0.00012
0.20	0.2000	0.0000	0.00012
0.50	0.5000	0.0000	0.00012
1.00	1.0000	0.0000	0.00012
2.00	2.0000	0.0000	0.00012
5.00	5.0000	0.0000	0.00012
10.00	10.0000	0.0000	0.00012
20.00	20.0001	-0.0001	0.00012
50.00	50.0000	0.0000	0.00014
100.00	100.0001	-0.0001	0.00019
200.00	200.0001	-0.0001	0.00032

### 5. OFF CENTER LOADING ERROR



POINT	READING (g)
1	100.0000
2	100.0000
3	100.0000
4	100.0000
5	100.0000
OFF-CENTER LOADING	0.0000

NOTE: THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR  $k=2$ , PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT





CERT.No.: HS-V015C

Calibration Date : 20 Mar 24  
 Submitted by : ASIA LAB @ CONSULTANT CO.,LTD  
 184 Soi Phutthamonthon Sai 2 Soi 12,  
 Bangphai, Bangkae, Bangkok 10160

Avg Room Temp : 20 °C  
 Avg Water Temp : 20 °C  
 Air Pressure : 760.00 mmHg  
 Salinity : 0 ppt

Model : YSI 5000  
 S/N : 15B100751  
 Probe : YSI 5010  
 S/N : 22D100097  
 ID NO. : -  
 Air Temp ref : S/N. F8065C26  
 Barometric ref : S/N. F8065C26  
 Water Temp ref : S/N. 11430  
 Technician : Kittipong M.

#### Calibration Details

Calibration Point	100% air sat. (@20 °C, DO = 9.09 mg/l)	(status)	(status)
Measurement 1 (mg/l)	9.08	(PASS)	-
Measurement 2 (mg/l)	9.08	(PASS)	-
Measurement 3 (mg/l)	9.08	(PASS)	-
Measurement 4 (mg/l)	9.08	(PASS)	-
Measurement 5 (mg/l)	9.08	(PASS)	-
Measurement 6 (mg/l)	9.08	(PASS)	-
Measurement 7 (mg/l)	9.08	(PASS)	-
Measurement 8 (mg/l)	9.08	(PASS)	-
Measurement 9 (mg/l)	9.08	(PASS)	-
Measurement 10 (mg/l)	9.08	(PASS)	-
Mean Measurement	9.08	mg/l	-
Inaccuracy	0.01	mg/l	-

Overall Status (PASS)

#### Manufacturer Specification

Accuracy = +/- 0.02 mg/l

- 1) This certificate is issued based on the result that are found as shown on date and place of test only.
- 2) The calibration procedure followed in accordance with Harikul Science Co., Ltd.
- 3) This result shall not be used for advertising purpose.



Technician Signature  
 (Kittipong Maekwong)



Laboratory Manager  
 (Supreecha Sumaritam)

CERT.No.: HS-W015C

Calibration Date : 18 Mar 25  
 Submitted by : S.P.S CONSULTING SERVICE CO.,LTD  
 7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol,  
 Chatuchak, Bangkok, Thailand 10900

Avg Room Temp : 20 °C  
 Avg Water Temp : 20 °C  
 Air Pressure : 760.00 mmHg  
 Salinity : 0 ppt

Model : YSI 5000  
 S/N : 15B100751  
 Probe : YSI 5010  
 S/N : 22D100097  
 ID NO. : -  
 Air Temp ref : S/N. F8065C26  
 Barometric ref : S/N. F8065C26  
 Water Temp ref : -  
 ID NO. HS001  
 Technician : Kittipong M.

#### Calibration Details

Calibration Point	100% air sat. (@20 °C, DO = 9.09 mg/l)	(status)	(status)
Measurement 1 (mg/l)	9.08	(PASS)	-
Measurement 2 (mg/l)	9.08	(PASS)	-
Measurement 3 (mg/l)	9.08	(PASS)	-
Measurement 4 (mg/l)	9.07	(PASS)	-
Measurement 5 (mg/l)	9.07	(PASS)	-
Measurement 6 (mg/l)	9.07	(PASS)	-
Measurement 7 (mg/l)	9.07	(PASS)	-
Measurement 8 (mg/l)	9.07	(PASS)	-
Measurement 9 (mg/l)	9.07	(PASS)	-
Measurement 10 (mg/l)	9.07	(PASS)	-

Mean Measurement	9.07	mg/l	-	-
Inaccuracy	0.02	mg/l	-	-

Overall Status (PASS)

#### Manufacturer Specification

Accuracy = +/- 0.02 mg/l

- 1) This certificate is issued based on the result that are found as shown on date and place of test only.
- 2) The calibration procedure followed in accordance with Harikul Science Co., Ltd.
- 3) This result shall not be used for advertising purpose.



Technician Signature  
 (Kittipong Maekwong)



Laboratory Manager  
 (Natenapha Pisatkunchon)





# QUALITY CALIBRATION CO.,LTD.

235 Petchkasem 63/2 Road, Laksong, Bangkai, Bangkok 10160

Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

[www.qcalibration.com](http://www.qcalibration.com)

CERTIFICATE No : 24T0774

REFERENCE No : 71986-2

PAGE : 1 OF 2

## Certificate of Calibration

**EQUIPMENT** : COD REACTOR

**MANUFACTURER** : HACH

**MODEL** : DRB 200

**SERIAL No** : 15110C0235

**ID No** : CRB 05/59

**SUBMITTED BY** : S.P.S. CONSULTING SERVICE CO., LTD.  
7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN RD.,  
JOMPOL, CHATUCHAK, BANGKOK 10900

**CALIBRATED BY** : CHAICHARN CH.

**CALIBRATION DATE** : 5-Feb-24

**APPROVED BY** :   
PONGSAK J.

**ISSUED DATE** : 5-Feb-24

**RECEIVED DATE** : 5-Feb-24





CERTIFICATE No : 24T0774

PAGE : 2 OF 2

## Calibration Report

EQUIPMENT : COD REACTOR  
MANUFACTURER : HACH  
ID NUMBER : CRB 05/59  
RECEIVED DATE : 5-Feb-24  
AMBIENT TEMPERATURE : 23° C ± 1° C

MODEL : DRB 200  
SERIAL NUMBER : 15110C0235  
CALIBRATION DATE : 5-Feb-24  
RELATIVE HUMIDITY : 52 %RH ± 10 % RH

### CONDITION OF THIS RESULTS OF CALIBRATION


1. THIS INSTRUMENT WAS CALIBRATED BY DIRECT MEASUREMENT TEMPERATURE RECORDER WITH THERMOCOUPLE TYPE K UNDER NO LOAD CONDITION. THE THERMOCOUPLES WERE PLACED ON 15 POINTS AND LOCATED ONE THERMOCOUPLE IN EACH OF THE FOUR CORNERS OF THE REACTOR AND PLACED THE EIGHTH THERMOCOUPLE AT THE CENTER OF THE REACTOR.

2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) DATA LOGGER WITH TC TYPE K	HYDRA 2635A	8009008	23T6640	14-Jul-24

3. THIS RESULT WAS FOUND ACCURATE AS SHOWN ON DATE AND PLACE OF CALIBRATION ONLY.  
4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.  
5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-  
- NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH QUALITY CALIBRATION CO.,LTD.

### RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

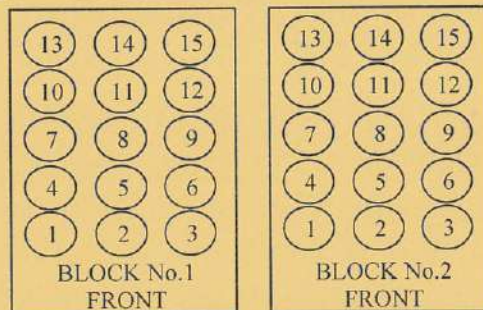

### TEMPERATURE MEASUREMENT ACCURACY TEST

Block No.	1	2
Controller temperature (°C)	145	145
Indicating Temperature	145	145
Measured Temperature (°C) at Spread Locations	1	150.2
	2	150.2
	3	150.2
	4	149.9
	5	150.1
	6	150.7
	7	149.9
	8	149.9
	9	150.8
	10	149.5
	11	150.2
	12	150.0
	13	149.5
	14	149.5
	15	149.6
Uncertainty of Measurement(± °C)	0.86	0.86

NOTE 1 : THE UNCERTAINTY OF MEASUREMENT EXCLUDED TEMPERATURE UNIFORMITY OF THE CHAMBER.

NOTE 2 : THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA.

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR k =2, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT





# QUALITY CALIBRATION CO., LTD.

235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160

Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

www.qcalibration.com

CERTIFICATE No : 25T0520

REFERENCE No : 75853-1

PAGE : 1 OF 2

## Certificate of Calibration

**EQUIPMENT** : COD REACTOR

**MANUFACTURER** : HACH

**MODEL** : DRB 200

**SERIAL No** : 15110C0497

**ID No** : DRB 05/59

**CONDITION AS RECEIVED** : USED ITEM

**SUBMITTED BY** : S.P.S. CONSULTING SERVICE CO., LTD.  
7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN RD.,  
JOMPOL, CHATUCHAK, BANGKOK 10900

**CALIBRATED BY** : CHAICHARN CH.

**CALIBRATION DATE** : 27-Jan-25

**APPROVED BY** :   
PONGSAK J.

**ISSUED DATE** : 27-Jan-25

**RECEIVED DATE** : 15-Jan-25

THIS CERTIFICATE MAY NOT BE REPRODUCED OTHER THAN IN FULL EXCEPT WITH THE PRIOR WRITTEN APPROVAL OF  
QUALITY CALIBRATION CO., LTD.



F-G010 REV : 03





# QUALITY CALIBRATION CO., LTD.

235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160

Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

CERTIFICATE No : 25T0520

PAGE : 2 OF 2

## Calibration Report

EQUIPMENT : COD REACTOR  
MANUFACTURER : HACH  
ID NUMBER : DRB 05/59  
RECEIVED DATE : 15-Jan-25  
AMBIENT TEMPERATURE : 23° C ± 1° C  
MODEL : DRB 200  
SERIAL NUMBER : 15110C0497  
CALIBRATION DATE : 27-Jan-25  
RELATIVE HUMIDITY : 53 %RH ± 10 % RH

### CONDITION OF THIS RESULTS OF CALIBRATION


1. THIS INSTRUMENT WAS CALIBRATED BY DIRECT MEASUREMENT METHOD WITH CALIBRATED THERMOCOUPLE TYPE K UNDER NO LOAD CONDITION. THE THERMOCOUPLES WERE PLACED ON POINTS AND LOCATED AS THE PICTURE.

2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) DATA LOGGER WITH TC TYPE K	HYDRA 2635A	6635300	24T6468	26-Jun-25

3. THE CERTIFICATE IS VALID FOR THE ITEM CALIBRATED AS SHOWN ON THE DATE AND PLACE OF CALIBRATION ONLY.  
4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.  
5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-  
- NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH QUALITY CALIBRATION CO., LTD.

### RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

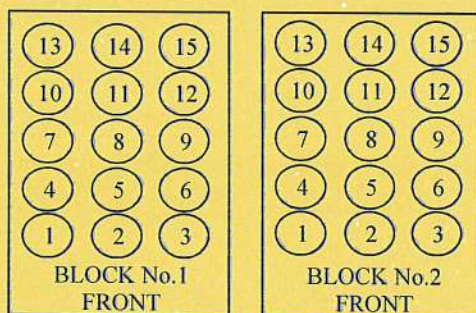

Block No.		1	2
Calibration Point (°C)		150	150
Controller temperature (°C)		144	144
Indicating Temperature		144	144
Measured Temperature (° C) at Spread Locations	1	150.01	149.57
	2	150.69	150.44
	3	150.40	149.46
	4	150.22	149.89
	5	150.27	149.75
	6	150.51	150.45
	7	150.24	150.03
	8	150.20	150.08
	9	150.14	150.14
	10	149.70	149.83
	11	149.58	149.89
	12	149.46	149.79
	13	148.77	149.03
	14	148.99	149.14
	15	149.02	149.62
Uncertainty of Measurement(± °C)		0.87	0.87

NOTE 1 : THE UNCERTAINTY OF MEASUREMENT EXCLUDED TEMPERATURE UNIFORMITY OF THE CHAMBER.

NOTE 2 : LOCATION 10 WAS REFERENCE LOCATION.

NOTE 3 : THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA.

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR k =2, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT







## MAINTENANCE AND TEST CERTIFICATE MODEL

### OPTIMA 5300DV

<b>Customer :</b> <u>S.P.S.Consulting Service Co.,Ltd</u>	Date Tested: <u>January 6, 2025</u>	
	Recommendation Recertification	
<b>Address :</b> <u>7 Soi Phaholyothin 24</u>	Period <u>6</u> Months	
<u>Paholyothin Road</u>	Recertification Due: <u>July 6, 2025</u>	
<u>Jompol Chatuchak, Bangkok 1090</u>	Date Last Certified: <u>July 4, 2024</u>	
<b>User Name:</b> <u>K.Phenpha Vipasthawatt</u>	Visit Number: <u>2 of 2</u>	
<b>Phone:</b> <u>083-9269252</u>	PerkinElmer Phone: <u>02-719-6420 ext 206</u>	
<b>Fax:</b> <u>02-513-4221</u>	PerkinElmer Fax: <u>02-318-5597</u>	

CONFIGURATION TESTED		ACCESSORIES/COMPONENT NOT INCLUDED
<b>MODEL</b>	<b>SERIAL NUMBER</b>	
<u>OPTIMA 5300DV</u>	<u>077C7042401</u>	
<b>TESTED EQUIPMENT</b>	<b>CALIBRATION NUMBER</b>	<b>EXPIRATION</b>
<u>IPV Methods</u>		
<b>TEST STANDARD USED</b>	<b>PART NUMBER</b>	<b>EXPIRATION DATE</b>
<u>Multielement Standard</u>	<u>N069-1579</u>	<u>December 30, 2025</u>
<u>Wavecal Solution</u>	<u>N058-2152</u>	<u>April 30, 2025</u>
<u>VIS Wavecal solution</u>	<u>N930-2946</u>	<u>December 30, 2025</u>
<u>Instrument Cal. STD4</u>	<u>N930-0221</u>	<u>August 30, 2025</u>
<b>CUSTOMER SUPPLIED</b>	<b>COMMENTS</b>	<b>CUSTOMER INITIALS</b>
<u>2 % HNO3</u>		
<u>10 % HNO3</u>		





## MAINTENANCE AND TEST CERTIFICATE MODEL

### OPTIMA 5300DV

**SERIAL NUMBER** 077C7042401**DATE TESTED** January 6, 2025**1. MECHANICAL CHECKS**

A. Inspect and clean all fans and filters.

☐ OK

B. Inspect and replace as necessary, all torch components including the RF coil.

☐ OK

C. Inspect all tubing for sign of clacking or leaking.

☐ OK

D. Adjust water and gas pressure regulator settings.

☐ OK

E. Inspect and leak check pneumatics drawers.

☐ OK

F. Clean the exterior of the instrument.

☐ OK**2. OPTICAL CHECKS**

A. Inspect and clean all optical components.

☐ OK

B. As required, check and replace all purgefilters.

☐ OK

C. Recheck optical alignment.

☐ OK**3. COOLING SYSTEM CHECKS**

A. Perform preventive maintenance on chiller.

☐ OK

B. Flush out the chiller every year.

☐ N/A**4. PERFORMANCE CHECKS**

A. Torch View Alignment.

☐ OK

B. Wavelength Calibration.

☐ OK



## MAINTENANCE AND TEST CERTIFICATE MODEL

### OPTIMA 5300DV

**SERIAL NUMBER :** 077C7042401
**DATE TESTED :** January 6, 2025

PARAMETER		SPECIFICATION		FINAL VALUE	
<b>Spectral Resolution : UV</b>	As 193.696 nm	≤ 0.007		0.00519	
	Ni 231.604 nm	≤ 0.008		0.00667	
	Ni 341.476 nm	≤ 0.012		0.00757	
<b>Spectral Resolution : VIS</b>	La 408.672 nm	≤ 0.020		0.01621	
	Ba 455.403 nm	≤ 0.025		0.02183	
<b>Precision</b>					
	As 193.656 nm	% RSD	< 1.0	0.51	%
	Zn 213.856 nm	% RSD	< 1.0	0.48	%
	Mn 257.610 nm	% RSD	< 1.0	0.03	%
	La 379.478 nm	% RSD	< 1.0	0.05	%
	Ba 455.403 nm	% RSD	< 1.0	0.07	%
	Ba 493.408 nm	% RSD	< 1.0	0.04	%
<b>Detection Limits : Axial</b>	Tl 190.080 nm	3(sd)		10.65	ppb
	As 193.696 nm	3(sd)		2.48	ppb
	Pb 220.353 nm	3(sd)		3.09	ppb
<b>Detection Limits : Radial</b>	As 193.696 nm	3(sd)		12.41	ppb
	Zn 213.856 nm	3(sd)		0.91	ppb
	Mn 257.610 nm	3(sd)		0.13	ppb
	La 379.478 nm	3(sd)		4.74	ppb
	Ba 455.403 nm	3(sd)		0.10	ppb
	Ba 493.408 nm	3(sd)		0.18	ppb
<b>BEC : Axial (IB X 500)/(IS-IB)</b>	Cd 226.502 nm	≤ 150 ppb		14.22	
<b>BEC : Radial (IB X 1000)/(IS-IB)</b>	Mn 257.610 nm	≤ 45 ppb		6.14	



## MAINTENANCE AND TEST CERTIFICATE MODEL

### OPTIMA 5300DV

SERIAL NUMBER 077C7042401DATE TESTED January 6, 2025**Remarks :**

Commissioning follow as commissioning performance sheets.

---

---

---

---

---

---

---

---

This is to certify that the above tests have been performed and the configuration tested



meets



does not meet

the PerkinElmer Specifications listed on this certificate.

This certificate does not modify PerkinElmer's standard terms and condition of sale,  
including warranty terms.

**Service Department PerkinElmer Ltd.****Authorized Representative:**

( Wiphan Promlumda )

Service Engineer





## MAINTENANCE AND TEST CERTIFICATE MODEL

### OPTIMA 5300DV

<b>Customer :</b> <u>S.P.S.Consulting Service Co.,Ltd</u>	<b>Date Tested:</b> <u>July 1, 2025</u>	
	<b>Recommendation Recertification</b>	
<b>Address :</b> <u>7 Soi Phaholyothin 24</u>	<b>Period</b> <u>6</u> <b>Months</b>	
<u>Paholyothin Road</u>	<b>Recertification Due:</b> <u>January 1, 2026</u>	
<u>Jompol Chatuchak, Bangkok 1090</u>	<b>Date Last Certified:</b> <u>January 6, 2025</u>	
<b>User Name:</b> <u>K.Phenpha Vipasthawatt</u>	<b>Visit Number:</b> <u>1 of 2</u>	
<b>Phone:</b> <u>083-9269252</u>	<b>PerkinElmer Phone:</b> <u>02-719-6420 ext 206</u>	
<b>Fax:</b> <u>02-513-4221</u>	<b>PerkinElmer Fax:</b> <u>02-318-5597</u>	

CONFIGURATION TESTED		ACCESSORIES/COMPONENT NOT INCLUDED
<b>MODEL</b>	<b>SERIAL NUMBER</b>	
<u>OPTIMA 5300DV</u>	<u>077C7042401</u>	
<b>TESTED EQUIPMENT</b>	<b>CALIBRATION NUMBER</b>	<b>EXPIRATION</b>
<u>IPV Methods</u>		
<b>TEST STANDARD USED</b>	<b>PART NUMBER</b>	<b>EXPIRATION DATE</b>
<u>Multielement Standard</u>	<u>N069-1579</u>	<u>December 30, 2024</u>
<u>Wavecal Solution</u>	<u>N058-2152</u>	<u>March 30, 2024</u>
<u>VIS Wavecal solution</u>	<u>N930-2946</u>	<u>February 28, 2024</u>
<u>Instrument Cal. STD4</u>	<u>N930-0221</u>	<u>November 30, 2024</u>
<b>CUSTOMER SUPPLIED</b>	<b>COMMENTS</b>	<b>CUSTOMER INITIALS</b>
<u>2 % HNO3</u>		
<u>10 % HNO3</u>		



## MAINTENANCE AND TEST CERTIFICATE MODEL

### OPTIMA 5300DV

**SERIAL NUMBER**    077C7042401

**DATE TESTED**    July 1, 2025

**1. MECHANICAL CHECKS**

- |  |                             |
|--|-----------------------------|
| A. Inspect and clean all fans and filters.                                       | <input type="checkbox"/> OK |
| B. Inspect and replace as necessary, all torch components including the RF coil. | <input type="checkbox"/> OK |
| C. Inspect all tubing for sign of clacking or leaking.                           | <input type="checkbox"/> OK |
| D. Adjust water and gas pressure regulator settings.                             | <input type="checkbox"/> OK |
| E. Inspect and leak check pneumatics drawers.                                    | <input type="checkbox"/> OK |
| F. Clean the exterior of the instrument.   | <input type="checkbox"/> OK |

**2. OPTICAL CHECKS**

- |   |                             |
|---|-----------------------------|
| A. Inspect and clean all optical components.        | <input type="checkbox"/> OK |
| B. As required, check and replace all purgefilters. | <input type="checkbox"/> OK |
| C. Recheck optical alignment.                       | <input type="checkbox"/> OK |

**3. COOLING SYSTEM CHECKS**

- |   |                              |
|---|------------------------------|
| A. Perform preventive maintenance on chiller. | <input type="checkbox"/> OK  |
| B. Flush out the chiller every year.          | <input type="checkbox"/> N/A |

**4. PERFORMANCE CHECKS**

- |                            |                             |
|----------------------------|-----------------------------|
| A. Torch View Alignment.   | <input type="checkbox"/> OK |
| B. Wavelength Calibration. | <input type="checkbox"/> OK |



## MAINTENANCE AND TEST CERTIFICATE MODEL

### OPTIMA 5300DV

**SERIAL NUMBER :** 077C7042401
**DATE TESTED :** July 1, 2025

PARAMETER		SPECIFICATION		FINAL VALUE	
<b>Spectral Resolution : UV</b>	<b>As</b>	<b>193.696 nm</b>	$\leq 0.007$	<u>0.00570</u>	
	<b>Ni</b>	<b>231.604 nm</b>	$\leq 0.008$	<u>0.00734</u>	
	<b>Ni</b>	<b>341.476 nm</b>	$\leq 0.012$	<u>0.00763</u>	
<b>Spectral Resolution : VIS</b>	<b>La</b>	<b>408.672 nm</b>	$\leq 0.020$	<u>0.01627</u>	
	<b>Ba</b>	<b>455.403 nm</b>	$\leq 0.025$	<u>0.02428</u>	
<b>Precision</b>					
	<b>As</b>	<b>193.656 nm</b>	% RSD < 1.0	<u>0.82</u>	%
	<b>Zn</b>	<b>213.856 nm</b>	% RSD < 1.0	<u>0.83</u>	%
	<b>Mn</b>	<b>257.610 nm</b>	% RSD < 1.0	<u>0.20</u>	%
	<b>La</b>	<b>379.478 nm</b>	% RSD < 1.0	<u>0.89</u>	%
	<b>Ba</b>	<b>455.403 nm</b>	% RSD < 1.0	<u>0.92</u>	%
	<b>Ba</b>	<b>493.408 nm</b>	% RSD < 1.0	<u>0.75</u>	%
<b>Detection Limits : Axial</b>	<b>Tl</b>	<b>190.080 nm</b>	3(sd)	<u>10.65</u>	ppb
	<b>As</b>	<b>193.696 nm</b>	3(sd)	<u>2.48</u>	ppb
	<b>Pb</b>	<b>220.353 nm</b>	3(sd)	<u>3.09</u>	ppb
<b>Detection Limits : Radial</b>	<b>As</b>	<b>193.696 nm</b>	3(sd)	<u>331.50</u>	ppb
	<b>Zn</b>	<b>213.856 nm</b>	3(sd)	<u>0.98</u>	ppb
	<b>Mn</b>	<b>257.610 nm</b>	3(sd)	<u>0.34</u>	ppb
	<b>La</b>	<b>379.478 nm</b>	3(sd)	<u>2.54</u>	ppb
	<b>Ba</b>	<b>455.403 nm</b>	3(sd)	<u>2.19</u>	ppb
	<b>Ba</b>	<b>493.408 nm</b>	3(sd)	<u>4.32</u>	ppb
<b>BEC : Axial (IB X 500)/(IS-IB)</b>	<b>Cd</b>	<b>226.502 nm</b>	$\leq 150$ ppb	<u>140.03</u>	
<b>BEC : Radial (IB X 1000)/(IS-IB)</b>	<b>Mn</b>	<b>257.610 nm</b>	$\leq 45$ ppb	<u>24.17</u>	





**MAINTENANCE AND TEST CERTIFICATE MODEL**  
**OPTIMA 5300DV**

**SERIAL NUMBER** 077C7042401

**DATE TESTED** July 1, 2025

**Remarks :**

Commissioning follow as commissioning performance sheets.

This is to certify that the above tests have been performed and the configuration tested



meets




does not meet

the PerkinElmer Specifications listed on this certificate.

This certificate does not modify PerkinElmer's standard terms and condition of sale,  
including warranty terms.

**Service Department PerkinElmer Ltd.**

**Authorized Representative:**



( Wiphan Promlumda )

Service Engineer

## MAINTENANCE REPORT AND CALIBRATION CERTIFICATE

### ATOMIC ABSORPTION SPECTROPHOTOMETER MODEL

PinAAcle 900T

<b>Customer :</b>	<u>S.P.S.Consulting Service Co.,Ltd</u>	<b>Date Tested:</b>	<u>January 6, 2025</u>
<b>Address :</b>	<u>7 Soi Phaholyothin 24</u>	<b>Recommendation Recertification</b>	
	<u>Paholyothin Road</u>	<b>Period</b>	<u>6</u> Months
	<u>Jompol Chatuchak, Bangkok 10900</u>	<b>Recertification Due:</b>	<u>July 6, 2025</u>
<b>User Name:</b>	<u>K.Phenpha Vipasthawatt</u>	<b>Date Last Certified:</b>	<u>July 4, 2024</u>
<b>Phone:</b>	<u>083-9269252</u>	<b>Visit Number:</b>	<u>1 OF 2</u>
<b>Email:</b>	<u></u>	<b>PerkinElmer Phone:</b>	<u>02-719-6420 ext 204</u>
		<b>PerkinElmer Fax:</b>	<u>02-318-5597</u>

CONFIGURATION TESTED		
MODEL	SERIAL NUMBER	SOFTWARE
<u>PinAAcle 900T</u>	<u>PTCS14111103</u>	<u>Wiblab V5.1</u>
<u>AS 900</u>	<u></u>	<u></u>
<u></u>	<u></u>	<u></u>
<u></u>	<u></u>	<u></u>
<u></u>	<u></u>	<u></u>
TEST STANDARD USED	PART NUMBER	EXPIRATION DATE
<u>Copper</u>	<u>N9300183</u>	<u>APR 30 2025</u>
<u>GFAAS Mixed standard</u>	<u>N9300244</u>	<u>FEB 28 2025</u>
<u>MG0-042</u>	<u>N101-3000</u>	<u></u>
<u>MG2-045</u>	<u>N101-3002</u>	<u></u>
<u></u>	<u></u>	<u></u>

## MAINTENANCE REPORT AND CALIBRATION CERTIFICATE

### ATOMIC ABSORPTION SPECTROPHOTOMETER MODEL

PinAAcle 900T

SERIAL NUMBER	PTCS14111103	DATE TESTED	January 6, 2025
<b>1. INSTRUMENT CHECKS</b>			
A. The Mirror and Lenses Condition			<input type="text" value="OK"/>
B. Grating Condition			<input type="text" value="OK"/>
C. Replace or Clean Dust Filter			<input type="text" value="OK"/>
D. Cleaning the Contact Cylinders			<input type="text" value="OK"/>
E. Cleaning the Furnace Windows			<input type="text" value="OK"/>
F. Cleaning the Burner Head			<input type="text" value="OK"/>
G. Cleaning the Nebulizer			<input type="text" value="OK"/>
H. Cleaning the Drain System			<input type="text" value="OK"/>
<b>2. AUTOSAMPLE CHECK</b>			
A. Sampling and Arm			<input type="text" value="OK"/>
B. Sampling & Rinse Pump			<input type="text" value="OK"/>
C. Sample Position & Clean			<input type="text" value="OK"/>
<b>3. COOLING SYSTEM CHECKS</b>			
A. Clean and Change Distill water			<input type="text" value="OK"/>
B. Themensor			<input type="text" value="OK"/>
<b>4. FIAS CHECKS</b>			
A. Pump and 5 Port Valve			<input type="text" value="N/A"/>
B. Chemifold and Tubing			<input type="text" value="N/A"/>
C. Power Supply			<input type="text" value="N/A"/>
D. Flow meter and Gas system			<input type="text" value="N/A"/>



## MAINTENANCE REPORT AND CALIBRATION CERTIFICATE

### ATOMIC ABSORPTION SPECTROPHOTOMETER MODEL

**PinAAcle 900T**

<b>SERIAL NUMBER</b>	<u>PTCS14111103</u>	<b>DATE TESTED</b>	<u>January 6, 2025</u>
<b>PARAMETER</b>		<b>SPECIFICATION</b>	<b>ACTUAL VAULE</b>
<b>A. Flame Mode Tests</b>			
1. Detector-Linearity with Barium (553.55 nm)			
Neutral Density Filter 0.2 :	<u>0.2042</u>	Abs. $\pm$ 5%	<u>0.2029</u> Abs.
Neutral Density Filter 1.0 :	<u>0.9798</u>	Abs. $\pm$ 5%	<u>1.0137</u> Abs.
2. Baseline Noise at 1 Abs with Barium (553.55 nm)			
(at an integration time of 0.5 seconds			
and 99 replicates)			
		SD $\leq$ 0.010 Abs.	<u>0.0016</u> Abs.
3. AA Baseline with Copper (Cu 324.75 nm)			
(at an integration time of 0.5 seconds			
and 99 replicates)			
		SD $\leq$ 0.001 Abs.	<u>0.0002</u> Abs.
4. D <sub>2</sub> Background Compensation (Copper 324.75 nm)			
with Neutral Density Filter 1.0		Absorbance $\leq$ 0.010 Abs	<u>0.0020</u> Abs.
5. AA-BG Baseline Noise with Copper (324.75 nm)			
(at an integration time of 2.0 seconds			
and 99 replicates)			
		SD $\leq$ 0.005 Abs.	<u>0.0002</u> Abs.
6. AA-BG Baseline Noise with Arsenic (193.70 nm)			
(at an integration time of 2.0 seconds			
and 99 replicates)			
		SD $\leq$ 0.005 Abs.	<u>0.0007</u> Abs.

## MAINTENANCE REPORT AND CALIBRATION CERTIFICATE

### ATOMIC ABSORPTION SPECTROPHOTOMETER MODEL

PinAAcle 900T

<b>SERIAL NUMBER</b>	<u>PTCS14111103</u>	<b>DATE TESTED</b>	<u>January 6, 2025</u>
<b>PARAMETER</b>	<b>SPECIFICATION</b>	<b>ACTUAL VAULE</b>	
7. Flame Interlock Shutdown	Shutdown correct?	<div>OK</div>	
8. Flame Sensitivity with Copper (324.75 nm)			
(5 mg/L Cu Standard a read time of 10 seconds			
10 replicates, standard burner and Stainless stell nebulizer)			
	Sensitivity $\geq 0.250$ Abs.	<u>0.3115</u>	Abs.
(2 mg/L Cu Standard a read time of 10 seconds			
10 replicates, standard burner and High sensitivity nebulizer)			
	Sensitivity $\geq 0.250$ Abs.	<u>N/A</u>	Abs.

## MAINTENANCE REPORT AND CALIBRATION CERTIFICATE

### ATOMIC ABSORPTION SPECTROPHOTOMETER MODEL

PinAAcle 900T

SERIAL NUMBER	PTCS14111103	DATE TESTED	January 6, 2025
PARAMETER	SPECIFICATION	ACTUAL VAULE	
B. THGA Tests			
1. Furnace Gas Flows			
Internal Flow	250 ± 25 mL/min	250	mL/min
External Flow	100 ± 10 mL/min	100	mL/min
2. Chromium Baseline Noise (357.87 nm)			
(mesure 5 furnace dry firings without any sample)			
	Baseline ≤ 0.005 Int.Abs	0.0012	
	SD ≤ 0.005 Int.Abs	0.0002	Int.Abs.
3. Chromium Characteristic Mass(m <sub>0</sub> ) and Precition (357.87 nm)			
(measure 5 furnace firing using 20 ul			
sample injections of 10 ug/L Cr standard)			
	m0 Results ≤ 7.0 pg/0.0044A-s	5.4	pg/0.0044A-s
	Precision ≤ 2.0%	1.15	%
4. Copper Characteristic Mass(m <sub>0</sub> ) and Zeeman Ratio (324.75 nm)			
(measure 5 furnace firing using 20 ul			
sample injections of 25 ug/L Cu standard)			
	m0 Results ≤ 16.5 pg/0.0044A-s	14.4	pg/0.0044A-s
	Zeeman Ratio 0.52 + 0.04	0.542	



## MAINTENANCE REPORT AND CALIBRATION CERTIFICATE

### ATOMIC ABSORPTION SPECTROPHOTOMETER MODEL

PinAAcle 900T

SERIAL NUMBER PTCS14111103 DATE TESTED January 6, 2025

Remarks :

- Neutral Density Filter refer to data sheet

- Zeeman Ratio =  $\frac{\text{Atomic Signal(peak area)}}{\text{Atomic Signal(peak area)+Background Signal(peak area)}}$   
= 0.1635/0.1635+0.1378  
0.542

This is to certify that the above tests have been performed and the configuration tested



meets




does not meet

the PerkinElmer Specifications listed on this certificate.

This certificate does not modify PerkinElmer's standard terms and condition of sale, including warranty terms.

**Service Department PerkinElmer Ltd.**

Customer Service Engineer:



( Wiphan Promlumda )

Service Engineer

**Cert. No. : SP24020**

**Pages 1 of 3**

## Calibration Certificate

**Equipment :** UV-VIS SPECTROPHOTOMETER  
**Manufacturer :** PERKINELMER  
**Model :** LAMBDA 25  
**Serial No.:** 501S14123010  
**ID No.:** SP03/58  
**Calibration Mode :** WAVELENGTH ACCURACY  
PHOTOMETRIC ACCURACY

**Condition As Found :** GOOD

**Customer :** S.P.S. CONSULTING SERVICE CO., LTD.  
7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN ROAD,  
CHOMPHON, CHATUCHAK,  
BANGKOK 10900, THAILAND.

**Location :** WET CHEMISTRY LABORATORY IV

**Ambient Temperature :** ( 28.1  $\pm$  5 ) °C  
**Relative Humidity :** ( 47.2  $\pm$  25 ) %

**Received Date :** 27 AUGUST 2024  
**Calibration Date :** 27 AUGUST 2024  
**Date of Issue :** 27 AUGUST 2024

**Calibrated by :**

Nathakorn Pisutpaisan

**Approved by :**

  
( Thanakul Petchurai )

# SITHIPORN ASSOCIATES CO., LTD.

## CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Banglumru, Bangplud, Bangkok, 10700 Thailand  
Tel. +66 2433 8331 Email : calibration@sithiporn.com

SITHIPORN  
associates



Cert. No. : SP24020

Job No. : VC67SP0013

Pages : 2 of 3

### Calibration Method :

This instrument was calibrated by using on-site calibration procedure In-house method : CP-SP-01

The calibration procedure to direct measurement wavelength accuracy by using wavelength standard solution, Photometric accuracy by using absorbance standard filter and absorbance standard solution

The calibration procedure used was based on ASTM E275-01, ASTM E925-02

### Condition of this result of calibration :

#### 1. Certified reference materials

Material	Ref. type	Cell serial No.	Cert. No.	Due Date
Holmium liquid	RM-HL	29706	106864	01/11/2024
Didymium liquid	RM-DL	28912	106905	02/11/2024
Neutral density filter	RM-1N2N3N	13877	106918	03/11/2024
Potassium dichromate solutions	RM-0204060810	14204	106902	02/11/2024
Potassium Iodide solution	-	KI-0701-001	CI-0185-24	14/05/2026

2. This result of calibration was found accurate as shown on date and place of calibration only.

3. This certificate is traceable to the international system of unit maintained at :

3.1 The UK National Physical Laboratory (NPL)

3.2 The National Institute of Standards and Technology, NIST.

### Result of calibration : Wavelength Accuracy

(Without adjustment)

Material	Certified Values of Reference Material (nm)	UUC* Reading (nm)	Error (nm)	Uncertainty ± (nm)	k Factor
RM-HL	278.13	278.3	0.17	0.16	2.00
	361.25	361.4	0.15	0.16	2.00
	467.82	467.7	-0.12	0.16	2.00
	536.56	536.5	-0.06	0.16	2.00
	640.50	640.4	-0.10	0.16	2.00
RM-DL	740.09	739.9	-0.19	0.16	2.00
	864.94	865.2	0.26	0.16	2.00

UUC\* = Unit Under Calibration

*G. Petch*



# SITHIPORN ASSOCIATES CO., LTD.

## CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbunru, Bangplud, Bangkok, 10700 Thailand  
Tel. +66 2433 8331 Email : calibration@sithiporn.com

SITHIPORN  
associates



Cert. No. : SP24020

Job No. : VC67SP0013

Pages : 3 of 3

### Result of calibration : Photometric Accuracy

(Without adjustment)

Material	Wavelength (nm)	Filter S/N	Nominal Absorbance (A)	Certified Absorbance (A)	UUC* Reading Absorbance (A)	Error (A)	Uncertainty ± (A)	k Factor
Neutral Density glass filter	440.0	29360	1.0	1.0517	1.0550	0.0033	0.0029	2.00
		29914	0.7	0.7445	0.7460	0.0015	0.0029	2.00
		29381	0.5	0.5416	0.5431	0.0015	0.0030	2.00
	546.1	29360	1.0	0.9821	0.9820	-0.0001	0.0028	2.00
		29914	0.7	0.6961	0.6958	-0.0003	0.0028	2.00
		29381	0.5	0.5073	0.5080	0.0007	0.0029	2.00
	590.0	29360	1.0	1.0222	1.0210	-0.0012	0.0028	2.00
		29914	0.7	0.7237	0.7221	-0.0016	0.0029	2.00
		29381	0.5	0.5361	0.5361	0.0000	0.0031	2.00
	635.0	29360	1.0	0.9753	0.9745	-0.0008	0.0028	2.00
		29914	0.7	0.6910	0.6900	-0.0010	0.0029	2.00
		29381	0.5	0.5211	0.5210	-0.0001	0.0032	2.00
Material	Wavelength (nm)	Solution (mg/l)	Certified Absorbance (A)	UUC* Reading Absorbance (A)	Error (A)	Uncertainty ± (A)	k Factor	
RM-0204060810	235.0	20	0.2422	0.2418	-0.0004	0.0101	2.00	
		40	0.4866	0.4852	-0.0014	0.0115	2.00	
		60	0.7414	0.7389	-0.0025	0.0067	2.00	
		80	0.9858	0.9842	-0.0016	0.0093	2.00	
		100	1.2442	1.2414	-0.0028	0.0086	2.00	

UUC\* = Unit Under Calibration

Condition of this result of calibration : Spectrophotometer PERKINELMER Model Lambda 25 S/N 501S14123010

Resolution of Wavelength Mode 0.1 nm

Resolution of Photometric Mode 0.0001 A

Parameter Setting

Measurement Mode Wavelength, Absorbance

Wavelength Scan 1100 nm-190 nm

Scanning Speed 7.5 nm/min

Data Pitch 0.1 nm

Band width(Wavelength) 1.0 nm

Band width(Vis) 1.0 nm

Band width(Uv) 1.0 nm

Stray Light\*\* UUC\* Reading at 220 nm

Transmission T(%)	Absorbance(A)
0.0117	3.8659

\*\*Specific Acceptance :

Transmission  $\leq$  1.0 T(%), Absorbance  $\geq$  2.0 A

\*\*Stray light not TISI Accredited


The reported uncertainty is based on a standard uncertainty multiplied by a coverage factor  $k$ , providing a level of confidence of approximately 95%

End of Calibration Certificate

*T. Ketch*

## ***Turbomass/Clarus Mass/ SQ8 MS Preventive Maintenance (PM)***

<b>Company Name:</b>	<b>S.P.S. Consulting Service Co.,Ltd</b>		
<b>Address (Instrument Location):</b>	7 Soi Phaholyothin24 Phaholyothin Road, Jompol, Chatuchak, Bangkok, 10900.		
<b>Serial Number:</b>	648N4050804	<b>PM Number:</b>	2 of 2
<b>Customer Name (if applicable):</b>	Ms. Naruecha	<b>Telephone Number:</b>	NA
<b>Service Engineer Name:</b>	Monchai Kitcharoenkeat	<b>Service Order Number:</b>	WO-02927336
<b>Date PM Performed: (DD-MMM-YYYY)</b>	22-Aug-2024	<b>Next PM Due Date: (DD-MMM-YYYY)</b>	22-Feb-2025

Part Number	Release	Publication Date	
TH09370064	C	March 2013	

### **Scope**

The purpose of this PM is to ensure the continued functionality of the Turbomass / Clarus MS SQ8 MS by inspecting and replacing any worn or damaged parts. This service should only be performed by a trained representative of PerkinElmer. The customer should save their method before the PM begins.

### **General Instructions:**

The customer must provide the engineer operational data to demonstrate recent instrument performance prior to starting the PM. Always check with the customer before making any changes that may affect the customer's analysis or calibration, including a current back-up of system software and/or data files. The completed document should be signed by an authorized PerkinElmer and customer representative and left with the customer. Update the PM sticker and instrument logbook as required.

### **Copyright Information**

This document contains proprietary information that is protected by copyright. All rights are reserved. No part of this publication may be reproduced in any form whatsoever or translated into any language without the prior, written permission of PerkinElmer, Inc **Copyright © 2013 PerkinElmer, Inc.**

### **Trademarks**

Registered names, trademarks, etc. used in this document, even when not specifically marked as such, are protected by law. PerkinElmer is a registered trademark of PerkinElmer, Inc. All other trademarks and registered trademarks not owned by PerkinElmer, Inc. or its subsidiaries that are depicted herein are the property of their respective owners. **Except as specifically set forth in its terms and conditions of sale, PerkinElmer makes no warranty of any kind with regard to this document, including, but not limited to, the implied warranties of merchantability and fitness for a particular purpose.** PerkinElmer shall not be liable for incidental or consequential damages in connection with the furnishing or use of this document.

## Component List

Component / Specific Model	Serial #	Software Version	Configuration Notes
Clarus680	680S14042502	Totalchrom6.3 <sup>+</sup>	PSS,PSS,FID
Clarus SQ8	648N4050804	Turbomass 6.4 <sup>+</sup>	
Atom X	US14113002	Tekma AtomX <sup>+</sup>	

## Parts lists

Parts Included with the PM				
Part Number (if applicable)	Description	Quantity	Batch/Lot #	Expiration Date (MM/YY)
N/A				

Additional Tools Required for PM				
Part Number (if applicable)	Description	Quantity	Serial #	Calibration Due Date (MM/YY)
N/A				
Additional Reagents and Standards Required for PM				
Part Number (if applicable)	Description	Quantity	Batch/Lot #	Expiration Date (MM/YY)
N/A				



## Procedure Checklist

Use ( x ) to check off those steps in the checklist that have been completed.

### General:

- ☒ Column type Elite 624.
- ☒ Carrier gas flow rate 1 ml/min.
- ☒ Review the instrument performance with the customer and document any recent problems.
- ☒ Inspect the customer log book and make any appropriate PM entries.
- ☒ Check incoming AC line voltage for proper levels and grounding.

### Mechanical:

- ☒ Inspect and clean all fans and filters.
- ☒ Check the level of FC-43 calibration compound in reference gas bulb and fill if necessary.
- ☒ Change the oil in the fore pump.
- ☒ Inspect cartridge in fore pump vacuum filter; replace adsorbent bead if necessary.
- ☒ Replace the exhaust vapor mist filter on the fore pump.
- ☒ Remove and clean the ion source assembly. Use the Insulator Replacement Kit and/or Optics Replacement Kit if necessary
- ☒ Replace the filament.
- ☒ Remove and clean the pre-quad rods.
- ☒ Observe Wide Range Gauge pressure; clean/adjust if required.
- ☒ Inspect and clean as needed all PC boards and bottom inside of MS chassis.

### Electrical:

- ☒ Check head amp offset. Adjust if necessary for proper value (Service Manual ).

### Operational Tests:

- ☒ Vacuum pressure.
- ☒ Air/water leak check
- ☒ AutoTune and mass calibration.
- ☒ Make a Chromatographic injection to verify peak shape and integrity only (not meant for sensitivity test).

### PC Maintenance:

- ☒ Delete all unnecessary temporary files.
- ☒ Empty deleted files from recycle bin.
- ☒ Perform hard drive defragmentation.

### Review:

- ☒ Review with the customer PM work performed.
- ☒ Review with the customer routine maintenance procedures.
- ☒ Discuss recommended customer-supplied materials to have on hand.

## Additional Comments


Additional Comments Regarding the PM

## Review

<b><i>The preventive maintenance checks and if applicable performance tests for Turbomass/ Clarus Mass/ SQ8 have been completed.</i></b>		
<b><i>This Turbomass/ClarusMS/SQ8      Pass                      the preventive maintenance.</i></b>		
<b>Review of Preventive Maintenance:</b>		
Authorized PerkinElmer Representative Monchai Kitcharoenkeat	Monchai	Date: 22-Aug-2024 (DD-MMM-YYYY)
Authorized Customer Representative: Ms. Naruecha	Narucha	Date: 22-Aug-2024 (DD-MMM-YYYY)

## ***GC Clarus 600/680 Preventive Maintenance (PM)***

<b>Company Name:</b>	<b>S.P.S. Consulting Service Co.,Ltd</b>		
<b>Address (Instrument Location):</b>	7 Soi Phaholyothin24 Phaholyothin Road, Jompol, Chatuchak, Bangkok, 10900.		
<b>Serial Number:</b>	680S14042502	<b>Service Tag:</b>	N68APSSFEMP
<b>Customer Name (if applicable):</b>	Ms.Naruecha	<b>PM number:</b>	1 of 2
<b>Service Engineer Name:</b>	Monchai Kitcharoenkeat	<b>Service Order Number:</b>	WO-
<b>Date PM Performed: (DD-MMM-YYYY)</b>	22-Feb-2025	<b>Next PM Due Date: (DD-MMM-YYYY)</b>	22-Aug-2025

<b>Part Number</b>	<b>Release</b>	<b>Publication Date</b>	
TH09370070	C	August 2016	

### **Scope**

The purpose of this PM is to ensure the continued functionality of the Clarus 600 and Clarus 680 GC by inspecting and replacing any worn or damaged parts. This service should only be performed by a trained representative of PerkinElmer. The customer should save their method before the PM begins.

### **General Instructions:**

The customer must provide the engineer operational data to demonstrate recent instrument performance prior to starting the PM. Always check with the customer before making any changes that may affect the customer's analysis or calibration, including a current back-up of system software and/or data files. The completed document should be signed by an authorized PerkinElmer and customer representative and left with the customer. Update the PM sticker and instrument logbook as required.

### **Copyright Information**

This document contains proprietary information that is protected by copyright. All rights are reserved. No part of this publication may be reproduced in any form whatsoever or translated into any language without the prior, written permission of Perkin Elmer, Inc. **Copyright © 2013 PerkinElmer, Inc.**

### **Trademarks**

Registered names, trademarks, etc. used in this document, even when not specifically marked as such, are protected by law. PerkinElmer is a registered trademark of PerkinElmer, Inc. All other trademarks and registered trademarks not owned by PerkinElmer, Inc. or its subsidiaries that are depicted herein are the property of their respective owners. **Except as specifically set forth in its terms and conditions of sale, PerkinElmer makes no Warranty of any kind with regard to this document, including, but not limited to, the implied warranties of merchantability and fitness for a particular purpose.** PerkinElmer shall not be liable for incidental or consequential damages in connection with the furnishing or use of this document.



## Component List

Component / Specific Model	Serial #	Software Version	Configuration Notes
Clarus680	680S14042502	Totalchrom6.3.2	PSS, PSS, FID,
Clarus SQ8T	648N4050804	Turbomass 6.4	
AtomX	US14113002	Tekma AtomX	

## Parts Lists

Additional Tools Required for PM				
Part Number (if applicable)	Description	Quantity	Serial #	Calibration Due Date (MM/YY)
N/A				
Additional Reagents and Standards Required for PM				
Part Number (if applicable)	Description	Quantity	Batch/Lot #	Expiration Date (MM/YY)
N/A				

## Procedure Checklist

Use (✓) to check off those steps in the checklist that have been completed.

### 1. General:

- ☒ Review the instrument performance with the customer and document any recent problems.

- ☒ Check incoming AC line voltage for proper levels and grounding.

L-N 220 Volt

L-G 220 Volt

N-G 0.33 Volt

*\*Neutral to ground not more than 0.5 volts peak to peak*

- ☒ Inspect all gas line filters and traps; Replace if necessary with customer supplied spares.

Carrier gas ☒ Helium ☐ Nitrogen ☐ Hydrogen

Moisture level ☒ Good ☐ Need to replace ☐ Other \_\_\_\_\_

Detector gas ☒ Air Zero ☒ Hydrogen ☐ Nitrogen ☐ Helium

Moisture level ☒ Good ☐ Need to replace ☐ Other \_\_\_\_\_

- ☒ Inspect the customer log book and make any appropriate PM entries.

- ☒ Leak check all fittings from the gas source to instrument.

Gas leakage ☒ Pass ☐ Fail Comment \_\_\_\_\_

- ☒ Perform general inspection of system for cleanliness.

- ☒ Inspect for functional and clean electronic cooling and oven vent fans

Electronic cooling fan ☒ Yes ☐ No

Oven cooling fan ☒ Yes ☐ No

### 2. Electronic :

- ☒ Check oven temperature. Calibrate if necessary.

Oven temperature set point 150 °C ☒ Pass ☐ Fail

- ☐ Check sub-ambient option. (If installed).

Oven temperature set point 5 °C ☐ Pass ☐ Fail

- ☒ Perform routine maintenance on detector/injector. Replace parts as necessary with customer supplied spares.

- ☒ Check flows, including split flows if applicable. Calibrate if necessary.
 

Carrier flow	Pass
Split flow	Pass
- ☒ Check detector gas flows and adjust if necessary.
 

Detector flow	Pass
---------------	------
- ☒ Autosampler installed ☒ Yes ☐ No
 

Check autosampler sensor for wear and replace if necessary.	
Vial sensor	Pass
Door sensor	Pass
Tower sensor	Pass
Plunger sensor	Pass
Elevator sensor	Pass
- ☒ Remove syringe, manually flush. Replace with customer supplied spare if necessary.
- ☒ Check firmware version. Upgrade to current levels if necessary.
 

Firmware version	<u>6.5</u>
------------------	------------
- ☒ Measure all accessible power supply voltages.
 

5 Volt	Pass
+15 Volt	Pass
-15 Volt	Pass
24 Volt	Pass
- ☒ Record all detector voltage signal.
 

Detector Channel A	<u>1.12</u>	mV.
Detector Channel B	<u>NA</u>	mV.

### 3. Diagnostics Tests:

- ☒ Run instrument diagnostics.
 

<input checked="" type="checkbox"/> BRAM	Pass
<input checked="" type="checkbox"/> EPROM	Pass
- ☒ Run Autosampler diagnostics.
 

<input checked="" type="checkbox"/> BRAM	Pass
<input checked="" type="checkbox"/> EPROM	Pass

### 4. Review:

- ☒ Review with the customer PM work performed.
- ☒ Review with the customer routine maintenance procedures.
- ☒ Discuss recommended customer-supplied materials to have on hand
- ☒ Attach PM sticker.
- ☒ Update Logbook.

## Additional Comments

Additional Comments Regarding the PM

## Review

<p><i>The preventive maintenance checks and if applicable performance tests for Clarus600/680 GC have been completed.</i></p>		
<p><i>This Clarus600/680 GC      Pass      the preventive maintenance.</i></p>		
<p><b>Review of Preventive Maintenance:</b></p>		
<p>Authorized PerkinElmer Representative:</p> <p>Monchai Kitcharoenkeat</p>	<p><i>Monchai</i></p>	<p>Date:</p> <p>22-Feb-2025 (DD-MMM-YYYY)</p>
<p>Authorized Customer Representative:</p> <p>Ms.Naruecha</p>	<p><i>Naruecha</i></p>	<p>Date:</p> <p>22-Feb-2025 (DD-MMM-YYYY)</p>



ลำดับที่ 4

ระดับเสียงในบรรยากาศ



THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-67/0304

MTC No. EEL. BP. 109/0267

## CALIBRATION CERTIFICATE

Submitted by : S.P.S.Consulting Service Co.,Ltd.

Address : 7 Soi Phaholyothin 24, Phaholyothin Road, Jompol, Chatuchak, Bangkok 10900.

Calibrated at : Electrical and Electronic Standards Laboratory, Industrial Metrology and Testing Service Centre.  
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Rd., Muang, Samutprakan 10280.

### Instrument Calibrated :

Description : Sound Calibrator

Manufacturer : ACO

Model : 2127

Serial No. : 130006

### Ambient Environment

Temperature :  $(23 + 3) ^\circ\text{C}$

Relative Humidity :  $(50 \pm 15) \%$

Ambient Pressure :  $(101.325 \pm 1.500) \text{ kPa}$

Standards used : 1. Digital Function Synthesizer NF Electronic DF-193A S/N 122037.

2. Measuring Amplifier Bruel&Kjaer 2636 S/N 1537484.

3. Programmable Attenuator Tamagawa TPA-303A S/N OF 2214.

4. Digital Multimeter Agilent 34401A S/N MY44005560.

5. Pressure Transmitter Vaisala PTB202AD S/N T0650001.

6. Audio Analyzer Keithley 2015-P S/N4106495.

7. Condenser Microphone B&K 4180 S/N 2889871.

**Calibration Procedure:** CP-102-04 based on IEC 60942-2003; The sound pressure level generated by sound calibrator under test shall be measured by standard microphone using an insert voltage technique.

This instrument has been calibrated against standards maintained at Electrical and Electronic Standards Laboratory (EEL), which are traceable to the International System of Units through the National Institute of Metrology (Thailand).

The information on actual reading is attached herewith and the uncertainty limits quoted refer to the measured values only.

Date of Receipt : 22 Feb. 2024

Date of Calibration : 4 Mar. 2024

1 / 2

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.4

#### Head Office

35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,  
Changwat Pathumthani 12120, Thailand

Tel. (66) 0 2577 9000

Fax. (66) 0 2577 9009

E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

#### Office/Laboratory

Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,  
Amphoe Muang, Changwat Samutprakan 10280, Thailand

Tel. (66) 0 2323 1672-80 ext. 115, 116

Fax. (66) 0 2323 9165

E-mail : mtc@tistr.or.th

#### Office

196 Phahonyothin Road, Chatuchak, Bangkok 10900,  
Thailand

Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217

Fax. (66) 0 2579 8592

E-mail : sumalee@tistr.or.th



Request No. 21-67/0304

MTC No. EEL. BP. 109/0267

The reported expanded uncertainty is based upon a standard uncertainty multiplied by a coverage factor  $k = 2$ , providing a level of confidence of approximately 95%.

Nominal Output of Unit Under Test = 94 dB re 20 $\mu$ Pa at 1000 Hz

Acoustic Output in dB re 20 $\mu$ Pa, Corrected to Reference Conditions: 101.325 kPa, 23.0 °C and 50 %RH.

1. Sound Pressure Level

Standard Microphone Type	Measured Sound Pressure Level (dB)	Deviated value (dB)	Uncertainty (dB)	Tolerance limit IEC60942:2003 Class 2
1/2 inch Bruel&Kjaer 4180	93.85	-0.15	$\pm 0.10$	$\pm 0.75$ dB

2. Frequency

Standard Microphone Type	Measured Frequency (Hz)	Deviated value (Hz)	Uncertainty (Hz)	Tolerance limit IEC60942:2003 Class 2
1/2 inch Bruel&Kjaer 4180	999.9	-0.1	$\pm 1.5$	$\pm 2.0\%$

3. Total Distortion


Standard Microphone Type	Measured Total Distortion (%)	Uncertainty (%)	Tolerance limit IEC60942:2003 Class 2
1/2 inch Bruel&Kjaer 4180	1.65	$\pm 0.50$	$\pm 4.0\%$

Note : 1. No adjustment.

2. The calibrator pressure correction was not included.

3. The microphone volume correction was not included.

Calibrated by :

  
.....  
(Mr. Weerachai Deechaiyae)

Approved by :

  
.....  
(Mr. Prawate Kluaypa)  
Director

Electrical and Electronic Standards Laboratory  
Industrial Metrology and Testing Service Centre

Date of Calibration : 4 Mar. 2024

Date of Issue : 5 Mar. 2024

Ref : 2011267022200795001

End of Certificate

2 / 2

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

Head Office

35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,  
Changwat Pathumthani 12120, Thailand  
Tel. (66) 0 2577 9000  
Fax. (66) 0 2577 9009  
E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

Office/Laboratory

Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,  
Amphoe Muang, Changwat Samutprakan 10280, Thailand  
Tel. (66) 0 2323 1672-80 ext. 115, 116  
Fax. (66) 0 2323 9165  
E-mail : mtc@tistr.or.th

Office

196 Phahonyothin Road, Chatuchak, Bangkok 10900,  
Thailand  
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217  
Fax. (66) 0 2579 8592  
E-mail : sumalee@tistr.or.th



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด  
S.P.S. CONSULTING SERVICE CO., LTD.  
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900  
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900  
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com., www.spscon.com

Noise R\_309/25

## Sound Level Meter Calibration Report

### Acoustic Calibrator Data

Brand	ACO	Number	AC 03/56
Model	2127	Serial No.	130006
Calibration Range	94 dB, 1000 Hz	Last Calibration	21 February 2025
		Due Date	21 February 2026

### Calibration Data

Sound Level Meter Data				Calibration Data		
SLM No.	Brand	Model	Serial No.	Date	Actual Reading [dB]	
					Before Adjustment	After Adjustment
ACO-R30	ACO	6236	00192042	18 May 2025	93.9	93.9
ACO-R33	ACO	6236	00192045	18 May 2025	93.9	93.9
ACO-R35	ACO	6236	00192047	18 May 2025	93.9	93.9
Acoustic Certified Value : Thailand Institute of Scientific and Technological Research (TISTR)					93.81 ± 0.10 dB	

Calibrated by :

Adul Dangklom  
(Mr. Adul Dangklom)

Approved by :

Peera Detudom  
(Mr. Peera Detudom)



ลำดับที่ 5

ระดับเสียงในสถานประกอบการ



THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-68/0220

MTC No. EEL. BP. 44/0268

## CALIBRATION CERTIFICATE

Submitted by : S.P.S.Consulting Service Co.,Ltd.

Address : 7 Soi Phaholyothin 24, Phaholyothin Road, Jompol, Chatuchak, Bangkok 10900.

Calibrated at : Electrical and Electronic Standards Laboratory, Industrial Metrology and Testing Service Centre.  
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Rd., Muang, Samutprakan 10280.

### Instrument Calibrated :

Description : Sound Calibrator

Manufacturer : ACO

Model : 2127

Serial No. : 130006

### Ambient Environment

Temperature :  $(23 \pm 3) ^\circ\text{C}$

Relative Humidity :  $(50 \pm 15) \%$

Ambient Pressure :  $(101.325 \pm 1.500) \text{ kPa}$

- Standards used :
1. Digital Function Synthesizer NF Electronic DF-193A S/N 122037.
  2. Measuring Amplifier Bruel&Kjaer 2636 S/N 1537484.
  3. Programmable Attenuator Tamagawa TPA-303A S/N OF 2214.
  4. Digital Multimeter Agilent 34401A S/N MY44005560.
  5. Pressure Transmitter Vaisala PTB202AD S/N T0650001.
  6. Audio Analyzer Panasonic VP-7722A S/N 041477D122.
  7. Condenser Microphone B&K 4180 S/N 2889871.

**Calibration Procedure:** CP-102-04 based on IEC 60942-2003; The sound pressure level generated by sound calibrator under test shall be measured by standard microphone using an insert voltage technique.

This instrument has been calibrated against standards maintained at Electrical and Electronic Standards Laboratory (EEL), which are traceable to the International System of Units through the National Institute of Metrology (Thailand).

The information on actual reading is attached herewith and the uncertainty limits quoted refer to the measured values only.

Date of Receipt : 19 Feb. 2025

Date of Calibration : 21 Feb. 2025

1 / 2  
W

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.5

#### Head Office

35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,  
Changwat Pathumthani 12120, Thailand  
Tel. (66) 0 2577 9036  
Fax. (66) 0 2577 9009

#### Office/Laboratory

668 Mu 2 Tambon Bangpoomai, Amphoe Muang Samutprakan,  
Changwat Samutprakan 10280, Thailand  
Tel. (66) 0 2323 1672-80 ext. 115, 116  
(66) 08 3219 9440  
E-mail : mtc@tistr.or.th Website : www.tistr.or.th

#### Office

196 Phahonyothin Road, Ladyao, Chatuchak,  
Bangkok 10900, Thailand  
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217  
(66) 08 1889 6827

THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-68/0220

MTC No. EEL. BP. 44/0268

The reported expanded uncertainty is based upon a standard uncertainty multiplied by a coverage factor  $k = 2$ , providing a level of confidence of approximately 95%.

Nominal Output of Unit Under Test = 94 dB re 20 $\mu$ Pa at 1000 Hz

Acoustic Output in dB re 20 $\mu$ Pa, Corrected to Reference Conditions: 101.325 kPa, 23.0 °C and 50 %RH.

1. Sound Pressure Level

Standard Microphone Type	Measured Sound Pressure Level (dB)	Deviated value (dB)	Uncertainty (dB)	Tolerance limit IEC60942:2003 Class 1
1/2 inch Bruel&Kjaer 4180	93.81	-0.19	$\pm 0.10$	$\pm 0.40$ dB

2. Frequency

Standard Microphone Type	Measured Frequency (Hz)	Deviated value (Hz)	Uncertainty (Hz)	Tolerance limit IEC60942:2003 Class 1
1/2 inch Bruel&Kjaer 4180	999.9	-0.1	$\pm 1.5$	$\pm 1.0\%$

3. Total Distortion

Standard Microphone Type	Measured Total Distortion (%)	Uncertainty (%)	Tolerance limit IEC60942:2003 Class 1
1/2 inch Bruel&Kjaer 4180	0.95	$\pm 0.50$	$\pm 3.0\%$

Note : 1. No adjustment.

2. The calibrator pressure correction was not included.

3. The microphone volume correction was not included.

Calibrated by :

  
(Mr. Weerachai Deechaiyae)

Approved by :

  
(Mr. Prawate Khuaypa)  
Director

Date of Calibration : 21 Feb. 2025

Date of Issue : 24 Feb. 2025

Electrical and Electronic Standards Laboratory  
Industrial Metrology and Testing Service Centre

Ref : 2011268021900739001

End of Certificate

2 / 2

The results relate only to the items tested/calibrated or value assigned.  
Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.5

Head Office  
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,  
Changwat Pathumthani 12120, Thailand  
Tel. (66) 0 2577 9036  
Fax. (66) 0 2577 9009

Office/Laboratory  
668 Mu 2 Tambon Bangpoomai, Amphoe Muang Samutprakan,  
Changwat Samutprakan 10280, Thailand  
Tel. (66) 0 2323 1672-80 ext. 115, 116  
(66) 08 3219 9440  
E-mail : mtc@tistr.or.th Website : www.tistr.or.th

Office  
196 Phahonyothin Road, Ladyao, Chatuchak,  
Bangkok 10900, Thailand  
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217  
(66) 08 1889 6827



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด  
S.P.S. CONSULTING SERVICE CO., LTD.  
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900  
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900  
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com., www.spscon.com

Noise R\_015/25

## Sound Level Meter Calibration Report

### Acoustic Calibrator Data

Brand	ACO	Number	AC 03/56
Model	2127	Serial No.	130006
Calibration Range	94 dB, 1000 Hz	Last Calibration	04 March 2024
		Due Date	04 March 2025

### Calibration Data

#### Sound Level Meter Data

#### Calibration Data

SLM No.	Brand	Model	Serial No.	Date	Actual Reading [dB]	
					Before Adjustment	After Adjustment
ACO-B41	ACO	6236	00192032	14 January 2025	93.9	93.9
ACO-R51	ACO	6236	00192063	14 January 2025	93.9	93.9
ACO-R52	ACO	6236	00192064	14 January 2025	93.9	93.9

Acoustic Certified Value : Thailand Institute of Scientific and Technological Research  
(TISTR)

93.85 ± 0.10 dB

Calibrated by :

Adul Dangklom  
(Mr. Adul Dangklom)

Approved by :

Peera Detudom  
(Mr. Peera Detudom)