

## เอกสารแนบ 6

---

เอกสารสอบเทียบเครื่องมือที่ใช้ในการ  
ตรวจวิเคราะห์



# CALIBRATION LABORATORY CO., LTD.

2/10-11, 14, 55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230  
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail: sale@cal-laboratory.com



## CERTIFICATE OF CALIBRATION

### FOR

NOMENCLATURE : BALANCE  
MANUFACTURER : METTLER TOLEDO  
MODEL / TYPE : MS204TS/00  
SERIAL NO. : B935191252[LA-002]  
CLID. NO. : 362200356  
JOB CONTROL NO. : 250215018254  
CALIBRATION SERVICE : ☐ IN-LABORATORY ☒ ON-SITE


CUSTOMER : ENVIRONMENTAL MEASUREMENTS CO., LTD.  
5/45 BAAN KLANG KRUNG BIZ TOWN, SOI SRINAGARINDRA 46/1 (PRAMOTE),  
NONG BON SUB-DISTRICT, PRAWET DISTRICT, BANGKOK 10250

DATE OF RECEIVED : 15 February 2025

DATE OF ISSUED : 04 March 2025

The report of calibration shall not be reproduced except in full without approval of the Calibration Laboratory Co., Ltd.

Calibrated By :

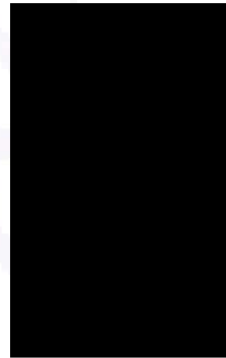

Approved By :

Authorized Signatory

04 March 2025

This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to the International System of Units (SI)

Certificate No. Q25018254

F3-011-05/12-23

page 1 of 3



@clcalibration



# CALIBRATION LABORATORY CO., LTD.

2/10-11, 14, 55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230  
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail: sale@cal-laboratory.com



## REPORT OF CALIBRATION

### FOR

NOMENCLATURE : BALANCE  
MANUFACTURER : METTLER TOLEDO  
MODEL / TYPE : MS204TS/00  
SERIAL NO. : B935191252[LA-002]  
LOCATION SITE : LABORATORY - BALANCE ROOM  
DATE OF CALIBRATION : 27 February 2025

#### ENVIRONMENT CONDITIONS :

Temperature : 23 °C to 24 °C

Relative Humidity : 49 % to 51 %

#### PROCEDURE USED :

This instrument was calibrated under procedure No. W1-305-46 based on EURAMET cg-18 Version 4.0 (11/2015).

The calibration was performed by Comparison with Weight Set which maintained by the Calibration Laboratory Co., Ltd.

#### REFERENCE STANDARD USED :

Weight Set, Mettler Toledo Class E2 S/N. 158850.

#### TRACEABILITY :

The measurements are traceable to International System of Units (SI), through National Institute of Metrology (Thailand).

Certificate No. MM-0165-23, Due Date 21 December 2025.

#### UNCERTAINTY :

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor complies with the table which for a normal distribution corresponds to a coverage probability of approximately 95%. It has been evaluated according to the "Evaluation of the Uncertainty of Measurement in Calibration (EA-4/02 M:2022)"

Certificate No. Q25018254

F3-011-05/12-23

page 2 of 3



@clcalibration

## CONDITION OF CALIBRATION ITEM : RECEIVED IN GOOD OPERATIONAL CONDITION

MEASUREMENT RESULTS : ( X ) without adjustment ( ) adjustment

### CALIBRATION DATA



#### 1. Error of indications

Nominal Test Value ( g )	Conventional mass ( g )	Display Value ( g )	Error of Balance ( g )	Uncertainty $\pm$ ( mg )	Coverage factor <i>k</i>
Unload	0.0000	0.0000	0.0000	0.06	2.00
0.1000	0.1000	0.1000	0.0000	0.14	2.00
0.5000	0.5000	0.5000	0.0000	0.15	2.00
1.0000	1.0000	1.0001	+0.0001	0.15	2.00
2.0000	2.0000	2.0001	+0.0001	0.15	2.00
5.0000	5.0000	5.0000	0.0000	0.15	2.00
10.0000	10.0000	10.0001	+0.0001	0.15	2.00

#### 2. Repeatability of indications

Nominal Test Value ( g )	Standard Deviation of Reading ( g )
200.0000	0.00004

#### 3. Effect of eccentric application of a load on the indication

					
	<input checked="" type="checkbox"/>				
Nominal Test Value ( g )	Display Value ( g )				
	Position 1	Position 2	Position 3	Position 4	Position 5
100.0000	99.9999	100.0001	99.9999	99.9998	99.9998
	Maximum Difference of Center Value ( g )				
	0.0002				

Note. The Scope of Accredited TISI Certificate No. 23-LB0092 Issue 02 Page 116 of 138

This report is valid for the above stated instrument/s only.

### End of Certificate ###

Certificate No. Q25018254

F3-011-05/12-23

page 3 of 3



@clcalibration

## CERTIFICATE OF CALIBRATION

### FOR

**NOMENCLATURE** : BALANCE  
**MANUFACTURER** : SHIMADZU  
**MODEL / TYPE** : AP225WD  
**SERIAL NO.** : D316300692[L/A-001]  
**CLID. NO.** : 362100172  
**JOB CONTROL NO.** : 250215018253  
**CALIBRATION SERVICE** : ☐ IN-LABORATORY ☒ ON-SITE

**CUSTOMER** : ENVIRONMENTAL MEASUREMENTS CO., LTD.


5/45 BAAN KLANG KRUNG BIZ TOWN, SOI SRINAGARINDRA 46/1 (PRAMOTE),  
NONG BON SUB-DISTRICT, PRAWET DISTRICT, BANGKOK 10250

DATE OF RECEIVED : 15 February 2025

DATE OF ISSUED : 04 March 2025

The report of calibration shall not be reproduced except in full without approval of the Calibration Laboratory Co., Ltd.

Calibrated By :



Approved By :

Authorized Signatory

04 March 2025

This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to the International System of Units (SI)

Certificate No. Q25018253

F3-011-05/12-23

page 1 of 3



@clcalibration



# CALIBRATION LABORATORY CO., LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230  
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



NSC-TISI-TIS 17025  
CALIBRATION 0059  
CLC

## REPORT OF CALIBRATION

### FOR

NOMENCLATURE : BALANCE  
MANUFACTURER : SHIMADZU  
MODEL / TYPE : AP225WD  
SERIAL NO. : D316300692[LA-001]  
LOCATION SITE : LABORATORY-BALANCE ROOM  
DATE OF CALIBRATION : 27 February 2025

#### ENVIRONMENT CONDITIONS :

Temperature : 23 °C to 24 °C  
Relative Humidity : 49 % to 51 %

#### PROCEDURE USED :

This instrument was calibrated under procedure No. WI-305-46 based on EURAMET/cg-18/Version 4.0 (11/2015).  
The calibration was performed by Comparison with Weight Set which maintained by the Calibration Laboratory Co., Ltd.

#### REFERENCE STANDARD USED :

Weight Set, Mettler Toledo Class E2 S/N. 158850.

#### TRACEABILITY :

The measurements are traceable to International System of Units (SI), through National Institute of Metrology (Thailand).  
Certificate No. MM-0165-23, Due Date 21 December 2025.

#### UNCERTAINTY :

The reported expanded uncertainty of measurement is stated as the standard uncertainty multiplied by the coverage factor complies with the table which for a normal distribution corresponds to a coverage probability of approximately 95%. It has been evaluated according to the "Evaluation of the Uncertainty of Measurement in Calibration (EA-4/02 M:2022)"

Certificate No. Q25018253

F3-011-05/12-23

page 2 of 3



@clcalibration



# CALIBRATION LABORATORY CO., LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230  
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



NSC-TISI-TIS 17025  
CALIBRATION 0059  
CLC

CONDITION OF CALIBRATION ITEM : RECEIVED IN GOOD OPERATIONAL CONDITION

MEASUREMENT RESULTS : (X) without adjustment ( ) adjustment

### CALIBRATION DATA

#### 1. Error of indications

Nominal Test Value (g)	Conventional mass (g)	Display Value (g)	Error of Balance (g)	Uncertainty ± (mg)	Coverage factor k
Unload	0.0000	0.0000	0.0000	0.07	2.00
5.0000	5.0000	5.0001	+0.0001	0.11	2.00
10.0000	10.0000	10.0000	0.0000	0.11	2.00
20.0000	20.0000	20.0000	0.0000	0.12	2.00
40.0000	40.0000	39.9999	-0.0001	0.14	2.00
60.0000	59.9999	59.9999	0.0000	0.15	2.00
80.0000	79.9999	80.0000	+0.0001	0.19	2.00
100.0000	99.9999	100.0000	+0.0001	0.17	2.00
120.0000	119.9999	120.0000	+0.0001	0.21	2.00
140.0000	139.9999	139.9999	0.0000	0.25	2.00
160.0000	159.9998	159.9998	0.0000	0.26	2.00
180.0000	179.9998	179.9998	0.0000	0.30	2.00
200.0000	199.9997	199.9996	-0.0001	0.26	2.00

#### 2. Repeatability of indications

Nominal Test Value (g)	Standard Deviation of Reading (g)
200.0000	0.00006

#### 3. Effect of eccentric application of a load on the indication

☐

☒

Nominal Test Value ( g )	Display Value ( g )	Maximum Difference of Center Value ( g )				
	Position 1	Position 2	Position 3	Position 4	Position 5	
100.0000	100.0000	99.9999	100.0000	100.0001	100.0000	0.0001

Note. The Scope of Accredited TISI Certificate No. 23-LB0092 Issue 02 Page 116,117 of 138

This report is valid for the above stated instrument/s only.

### End of Certificate ###

Certificate No. Q25018253

F3-011-05/12-23

page 3 of 3



@clcalibration



**CALIBRATION LABORATORY Co., LTD.**  
2/10-11, 14, 55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230  
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail: sale@cal-laboratory.com



## CERTIFICATE OF CALIBRATION

### FOR

NOMENCLATURE : DO METER  
MANUFACTURER : YSI  
MODEL / TYPE : 5000-230V/5010  
SERIAL NO. : 16D10162  
CLID. NO. : 272100329  
JOB CONTROL NO. : 250410042960  
CALIBRATION SERVICE : ☒ IN-LABORATORY ☐ ON-SITE


CUSTOMER : ENVIRONMENTAL MEASUREMENTS CO., LTD.  
5/45 BAAN KLANG KRUNG BIZ TOWN, SOI SRINAGARINDRA 46/1 (PRAMOTE),  
NONG BON SUB-DISTRICT, PRAWET DISTRICT, BANGKOK 10250

DATE OF RECEIVED : 10 April 2025

DATE OF ISSUED : 18 April 2025

The report of calibration shall not be reproduced except in full without approval of the Calibration Laboratory Co., Ltd.

Calibrated By :



Approved By :

Authorized Signatory

18 April 2025

This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to the International System of Units (SI)

Certificate No. Q25042960

F3-011-05/12-23

page 1 of 3

F3-011-05/12-23

page 2 of 3

Certificate No. Q25042960

## REPORT OF CALIBRATION

### FOR

NOMENCLATURE : DO METER  
MANUFACTURER : YSI  
MODEL / TYPE : 5000-230V/5010  
SERIAL NO. : 16D101626/19D100367[DOM-01]  
DATE OF CALIBRATION : 11 April 2025

### ENVIRONMENT CONDITIONS :

Temperature :  $(25 \pm 2.5) ^\circ\text{C}$  Relative Humidity :  $(50 \pm 15) \% \text{RH}$

### PROCEDURE USED :

This instrument was calibrated under procedure No. CLC-CPCH-06. The calibration was performed by direct measurement with Certified Reference Material (CRM).

### REFERENCE STANDARD USED :

Dissolved Oxygen, Sigma-Aldrich Product ID QC3077-500ML.

### TRACEABILITY :

The measurements are traceable to International System of Units (SI), through Merck Co., Ltd.  
Lot LRAD8571, Due Date April 2026.

### UNCERTAINTY :

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor  $k = 2.00$  which for a normal distribution corresponds to a coverage probability of approximately 95 %. It has been evaluated according to the "Evaluation of the Uncertainty of Measurement in Calibration (EA-4/02 M:2022)"







**CONDITION OF CALIBRATION ITEM : RECEIVED IN GOOD OPERATIONAL CONDITION  
MEASUREMENT RESULTS : ( X ) without adjustment ( ) adjustment**

The table in the following gives the calibration results and associated measurement uncertainties of Do Meter.

**CALIBRATION DATA**

**DO METER RESULT @ 20 °C**

Nominal Value ( mg/L )	DUC Reading ( mg/L )	Correction ( mg/L )	Uncertainty ( mg/L )
8.18	8.2	-0.02	± 0.38

Note. The Scope of Accredited ANAB Certificate No. ACDM-2814 Version 01.5 Page 5 of 68

This report is valid for the above stated instrument/s only.

### End of Certificate ###



**CERTIFICATE OF CALIBRATION**

**FOR**

NOMENCLATURE : HOT AIR OVEN  
MANUFACTURER : MEMMERT  
MODEL / TYPE : UF110  
SERIAL NO. : B422.0026[LA-0012]  
CLID. NO. : 332202464  
JOB CONTROL NO. : 250306027140  
CALIBRATION SERVICE : ☐ IN-LABORATORY ☒ ON-SITE

CUSTOMER : ENVIRONMENTAL MEASUREMENTS CO., LTD.  
5/45 BAAN KLANG KRUNG BIZ TOWN, SOI SRINAGARINDRA 46/1 (PRAMOTE),  
NONG BON SUB-DISTRICT, PRAWET DISTRICT, BANGKOK 10250

DATE OF RECEIVED : 06 March 2025

DATE OF ISSUED : 25 March 2025

The report of calibration shall not be reproduced except in full without approval of the Calibration Laboratory Co., Ltd.

Calibrated By :



Approved By :

Authorized Signatory

25 March 2025

This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to the International System of Units ( SI )





**CALIBRATION LABORATORY CO., LTD.**  
2/10-11,14, 55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230  
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



**CALIBRATION LABORATORY CO., LTD.**  
2/10-11,14, 55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230  
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com

## REPORT OF CALIBRATION

### FOR

NOMENCLATURE : HOT AIR OVEN  
MANUFACTURER : MEMMERT  
MODEL / TYPE : UF110  
SERIAL NO. : B422.0026[LA-0012]  
LOCATION SITE : LABORATORY-HOT ZONE  
DATE OF CALIBRATION : 19 March 2025

#### ENVIRONMENT CONDITIONS :

Temperature : 24 °C to 25 °C

Relative Humidity : 49% to 51 %

#### PROCEDURE USED :

This instrument was calibrated under procedure No. CLC-CPTH-07 based on TLAS G-20 as calibration guidelines.  
The calibration was performed by using Hydra Data Logger which maintained by the Calibration Laboratory Co., Ltd.

#### REFERENCE STANDARD USED :

Hydra Data Logger, Fluke Model 2620 S/N: 5592550.

#### TRACEABILITY :

The measurements are traceable to International System of Units (SI), through Calibration Laboratory Co., Ltd.  
Certificate No. Q24052150, Due Date 27 May 2025.

#### UNCERTAINTY :

The reported expanded uncertainty of measurement is stated as the standard uncertainty multiplied by the coverage factor complies with the table which for a normal distribution corresponds to a coverage probability of approximately 95 %.  
It has been evaluated according to the "Evaluation of the Uncertainty of Measurement in Calibration (EA-4/02 M:2022)"

Certificate No. Q25027140

F3-011-05/12-23



page 2 of 4

Certificate No. Q25027140

F3-011-05/12-23



page 3 of 4



# CALIBRATION LABORATORY Co., LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230  
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



ISO/IEC 17025


## CALIBRATION DATA

### 2. TEMPERATURE DISTRIBUTION

DUC	Setting ( ° C )	Measured Temperature ( ° C )@Probe No.9 is Ref.									Uncertainty ± ( ° C )	Coverage factor k
		1	2	3	4	5	6	7	8	9		
104.0	104.0	103.64	103.91	103.49	103.54	103.67	103.61	103.47	103.96	103.72	0.43	2,00
180.0	180.0	179.19	179.91	178.87	179.17	179.38	179.38	178.90	179.22	179.63	0.51	2,00

Technical Note : W = 56 cm, D = 40 cm, H = 48 cm.

Note. The Scope of Accredited ANAB Certificate No. ACDM-2814 Version 015 Page 59 of 68

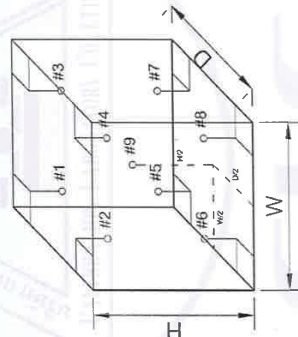

This report is valid for the above stated instrument/s only.

### End of Certificate ###

Certificate No. Q25027140

F3-011-05/12-23

page 4 of 4



@clcalibration



# CALIBRATION LABORATORY Co., LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230  
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



## CERTIFICATE OF CALIBRATION

### FOR

NOMENCLATURE : INCUBATOR  
MANUFACTURER : ACCUPLUS  
MODEL / TYPE : SMART i250  
SERIAL NO. : 2059-0718-0010[LA-002]  
CLID. NO. : 332100155  
JOB CONTROL NO. : 250215018255  
CALIBRATION SERVICE : ☐ IN-LABORATORY ☒ ON-SITE

CUSTOMER : ENVIRONMENTAL MEASUREMENTS CO., LTD.

5/45 BAAAN KLANG KRUNG BIZ TOWN, SOI SRINAGARINDRA 46/1 (PRAMOTE),  
NONG BON SUB-DISTRICT, PRAWET DISTRICT, BANGKOK 10250

DATE OF RECEIVED : 15 February 2025

DATE OF ISSUED : 04 March 2025

The report of calibration shall not be reproduced except in full without approval of the Calibration Laboratory Co., Ltd.

Calibrated By :



Approved By :

Authorized Signatory

04 March 2025

This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to the International System of Units (SI)

Certificate No. Q25018255

F3-011-05/12-23

page 1 of 4



@clcalibration



# REPORT OF CALIBRATION

## FOR

NOMENCLATURE : INCUBATOR  
MANUFACTURER : ACCUPLUS  
MODEL / TYPE : SMART i250  
SERIAL NO. : 2059-0718-0010[LA-002]  
LOCATION SITE : LABORATORY  
DATE OF CALIBRATION : 27 February 2025

### ENVIRONMENT CONDITIONS :

Temperature : 24 °C to 25 °C  
Relative Humidity : 49 % to 51 %

### PROCEDURE USED :

This instrument was calibrated under procedure No. WI-305-165 based on TLAS G-20-1/02-08 as calibration guidelines.  
The calibration was performed by using Hydra Series II which maintained by the Calibration Laboratory Co., Ltd.

### REFERENCE STANDARD USED :

Hydra Series II, Fluke Model 2635A S/N: 8209003.

### TRACEABILITY :

The measurements are traceable to International System of Units (SI), through Calibration Laboratory Co., Ltd.  
Certificate No. Q24052151, Due Date 27 May 2025.

### UNCERTAINTY :

The reported expanded uncertainty of measurement is stated as the standard uncertainty multiplied by the coverage factor complies with the table which for a normal distribution corresponds to a coverage probability of approximately 95 %.  
It has been evaluated according to the "Evaluation of the Uncertainty of Measurement in Calibration (EA-4/02 M:2022)"

Certificate No. Q25018255

F3-011-05/12-23



## CONDITION OF CALIBRATION ITEM : RECEIVED IN GOOD OPERATIONAL CONDITION

### MEASUREMENT RESULTS : ( X ) without adjustment ( ) adjustment

The table in the following gives the calibration results and associated measurement uncertainties of the measuring incubator.

#### CALIBRATION DATA

##### 1. INCUBATOR PERFORMANCE

DUC		Measured Uniformity ( °C )	Measured Stability ( °C )	Measured Overall Variation ( °C )
Setting ( °C )	Indicating ( °C )			
20.0	20.0	0.43	0.34	0.98

Certificate No. Q25018255

F3-011-05/12-23






CALIBRATION DATA

2. TEMPERATURE DISTRIBUTION

DUC		Measured Temperature ( °C )@Probe No.9 is Ref.									Uncertainty ± ( °C )	Coverage factor <i>k</i>
Setting ( °C )	Indicating ( °C )	1	2	3	4	5	6	7	8	9		
20.0	20.0	20.55	20.53	20.57	20.51	20.59	20.52	20.40	20.47	20.27	0.58	2.00

Technical Note : W = 50 cm, D = 48 cm, H = 110 cm.

The Scope of Accredited TISI Certificate No. 23-LB0092 Issue 02 Page 129 of 138

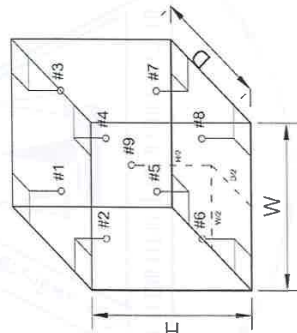

This report is valid for the above stated instrument/s only.

### End of Certificate ###



CERTIFICATE OF CALIBRATION

FOR


NOMENCLATURE : pH METER  
MANUFACTURER : APERA  
MODEL / TYPE : PH700/201T-F  
SERIAL NO. : PH700X1019061009/N/A [LA-008/PH-02]  
CLID. NO. : 272401000  
JOB CONTROL NO. : 250410042961  
CALIBRATION SERVICE : ☒ IN-LABORATORY ☐ ON-SITE

CUSTOMER : ENVIRONMENTAL MEASUREMENTS CO., LTD.  
5/45 BAAN KLANG KRUNG BIZ TOWN, SOI SRINAGARINDRA 46/1 (PRAMOTE),  
NONG BON SUB-DISTRICT, PRAWET DISTRICT, BANGKOK 10250

DATE OF RECEIVED : 10 April 2025 DATE OF ISSUED : 18 April 2025

The report of calibration shall not be reproduced except in full without approval of the Calibration Laboratory Co., Ltd.

Calibrated By :



Approved By :



Authorized Signatory

18 April 2025

This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to the International System of Units (SI)





# CALIBRATION LABORATORY CO., LTD.

2/10-11, 14, 55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230  
Tel: 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com Email:sae@cal-laboratory.com



## REPORT OF CALIBRATION

### FOR

NOMENCLATURE : pH METER  
MANUFACTURER : APERA  
MODEL / TYPE : PH700/201T-F  
SERIAL NO. : PH700X1019061009/N/A [LA-008/PH-02]  
DATE OF CALIBRATION : 11 April 2025

#### ENVIRONMENT CONDITIONS :

Temperature :  $(25 \pm 2.5) ^\circ\text{C}$  Relative Humidity :  $(50 \pm 15) \% \text{ RH}$

#### PROCEDURE USED :

This instrument was calibrated under procedure No. WI-305-128, 238. The calibration was performed by direct measurement with Certified Reference Material (CRM) and comparison with Calibration Bath, Precision Thermometer and IPRT which maintained by the Calibration Laboratory Co., Ltd.

#### REFERENCE STANDARD USED :

1. pH Standard Solution, NIMT TRM CODE TRM-S-2003, TRM CODE TRM-S-2007.
2. pH Standard Solution, Control Company Catalog Number 06664260, 11754256, Lot Number CC787362.
3. Calibration Bath, Kambic Model OB-222 ULT S/N. 17115653.
4. Precision Thermometer, ASL Model F250 S/N. 1334023800.
5. IPRT, Wika Model CTP5000-250-D S/N. PO00043543-1-10-1.

Certificate No. Q25042961

F3-011-05/12-23

page 2 of 4



@clcalibration



# CALIBRATION LABORATORY CO., LTD.

2/10-11, 14, 55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230  
Tel: 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com Email:sae@cal-laboratory.com



#### TRACEABILITY :

1. The measurements are traceable to International System of Units (SI), through National Institute of Metrology (Thailand), Lot Number: 080124, 120124, Due Date 23 January 2026.
2. The measurements are traceable to International System of Units (SI), through Control Company, Certificate No. 4281-14495731, Due Date 27 September 2025.
3. The measurements are traceable to International System of Units (SI), through Calibration Laboratory Co., Ltd., Certificate No. Q24120999, Due Date 26 November 2025.
4. The measurements are traceable to International System of Units (SI), through Thailand Institute of Scientific and Technological Research (TISTR), Certificate No. PSL-T 1042/67, Due Date 16 October 2025.
5. The measurements are traceable to International System of Units (SI), through National Institute of Metrology (Thailand), Certificate No. TT-0146-24, Due Date 28 October 2025.

#### UNCERTAINTY :

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor complies with the table which for a normal distribution corresponds to a coverage probability of approximately 95 %.

It has been evaluated according to the "Evaluation of the Uncertainty of Measurement in Calibration (EA-4/02 M:2022)"

Certificate No. Q25042961

F3-011-05/12-23

page 3 of 4



@clcalibration



# CALIBRATION LABORATORY CO., LTD.

2/10-11, 14, 55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230  
Tel: 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com Email: sale@cal-laboratory.com



## CONDITION OF CALIBRATION ITEM : RECEIVED IN GOOD OPERATIONAL CONDITION

### MEASUREMENT RESULTS : ( X ) without adjustment ( ) adjustment

The table in the following gives the calibration results and associated measurement uncertainties of pH meter.

#### CALIBRATION DATA

##### 1. pH METER RESULT @ 25 °C

Standard pH Buffer Solution (pH)	pH Meter Reading (pH)	pH Meter Reading (mV)	Correction (pH)	Uncertainty of Measurement (± pH)	k Factor
4.003	4.01	134	-0.007	0.014	2.00
7.005	7.00	-43	+0.005	0.014	2.00
10.015	10.01	-208	+0.005	0.100	2.05

Technical Note. Setting function CAL 3 point ( 4,7,10 ).

Note. The Scope of Accredited TISI Certificate No. 23-LB0092 Issue 02 Page 91 of 138

##### \*2. TEMPERATURE RESULT

Immersion depth (mm)	Actual Temperature (°C)	DUC Reading (°C)	Correction (°C)	Uncertainty ± (°C)
100	25.01	24.9	+0.11	0.07

Technical Note. Type of sensor : pH Probe

Probe Ø 12 mm

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor of  $k = 2.00$ .

Note. \* means Calibrations marked " Not TISI Accredited " in this Certificate have been included for completeness.

This report is valid for the above stated instrument/s only.

### End of Certificate ###

Certificate No. Q25042961

F3-011-0512-23

page 4 of 4



# SP METROLOGY SYSTEM ( THAILAND ) CO., LTD.

a Trescal company



ID LINE : IEC17025

## Certificate of Calibration

Certificate Number : SPR25050011-3

Page : 1 of 3

Customer : ENVIRONMENTAL MEASUREMENTS CO., LTD.

5/45 Baan Klang Krung Biz Town, Soi Srinagarindra 46/1 (Pramote),

Nongbon Sub-district, Prawet District, Bangkok 10250

Equipment Name : Refrigerator  
Manufacturer : Medicoool  
Model : BB-117  
Serial Number : BB117-190725001  
ID. Number : LA-003

#### Environmental Conditions

Ambient Temperature :  $25\text{ }^{\circ}\text{C} \pm 10\text{ }^{\circ}\text{C}$  Received Date : 02 May 2025  
Relative Humidity :  $60\% \pm 20\%$  Calibration Date : 06 May 2025  
Location of Calibration : On-Site Recommend Due Date : N/A  
Calibration Procedure : SP-CPT-04-01 Date of Issue : 07 May 2025

#### Method of Calibration

This certifies that the above instrument was calibrated in compliance with the calibration system requirement of ISO/IEC 17025:2017 in accordance with reference procedure. Standards used to perform this calibration are certified by to NIST or equivalent, National metrology institute, Natural physical constants, consensus standards. The result reported herein apply only to the calibration of the item described above as received. Our decision rule is to contact the customer if the item pass and fail calibration when the results include the uncertainties and the customer must determine if the results meets their needs. The calibration certificate shall not be reproduced except in full, without written approval of SP Metrology System (Thailand).

Calibrated by :

Approved by

Authorized Signatory

SP-FM-04-15 rev.0



## Calibration Report

Certificate Number : SPR25050011-3

Page : 2 of 3

### Reference Standards

Equipment Name	Model	Serial No.	Certificate No.	Due. Date
Data Acquisition/Switch Unit	34970A	MY44074688	SPR24080102-24	07 Sep 2025

### Traceability

This certification is traceable to the International System of Unit maintained at :  
 SP Metrology - SP Metrology system (Thailand) Co.Ltd.




ID LINE : IEC17025

## Result of Calibration

Certificate Number : SPR25050011-3

Page : 3 of 3

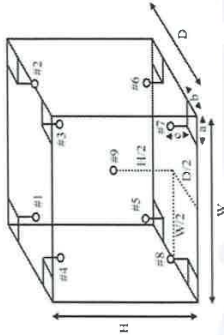

Temperature Accuracy in the Measurement Zone.

UUC Setting	Measured Temperature (°C) @ Probe No. 9 is REF.)									Uncertainty ( ± )
	# 1	# 2	# 3	# 4	# 5	# 6	# 7	# 8	# 9	
4.0	3.37	4.12	4.25	4.13	3.93	3.98	3.95	4.23	4.16	0.60

Unit : °C

Temperature Uniformity, Stability, Overall Variation

Unit : °C

UUC Setting	UUC Reading	Temperature Stability	Temperature Uniformity	Overall Variation
4.0	4.0	0.09	0.94	1.07

### Note :

The result of calibration was found accurate as show on date and place of calibration only.  
 This Certificate is not certified for any commercial transaction.

### Measurement Uncertainty

The reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor  $k = 2$ , providing a level of confidence approximately 95 %

- End of Certificate -





## CERTIFICATE OF CALIBRATION

### FOR


NOMENCLATURE : DIGITAL THERMOMETER WITH PROBE  
MANUFACTURER : LUTRON  
MODEL / TYPE : MTM-380SD  
SERIAL NO. : I.570147/N/A[LA-0013/LA-0013/A]  
CLID. NO. : 232204019  
JOB CONTROL NO. : 250408041416  
CALIBRATION SERVICE : ☒ IN-LABORATORY ☐ ON-SITE

CUSTOMER : ENVIRONMENTAL MEASUREMENTS CO., LTD.  
5/45 BAAN KLANG KRUNG BIZ TOWN, SOI SRINAGARINDRA 46/1 (PRAMOTE),  
NONG BON SUB-DISTRICT, PRAWET DISTRICT, BANGKOK 10250

DATE OF RECEIVED : 08 April 2025 DATE OF ISSUED : 11 April 2025

The report of calibration shall not be reproduced except in full without approval of the Calibration Laboratory Co., Ltd.

Calibrated By :



Approved By :

Authorized Signatory  
11 April 2025

This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to the International System of Units (SI)

Certificate No. Q25041416  
F3-011-05/12-23

page 1 of 3



@clcalibration



## REPORT OF CALIBRATION

### FOR

NOMENCLATURE : DIGITAL THERMOMETER WITH PROBE  
MANUFACTURER : LUTRON  
MODEL / TYPE : MTM-380SD  
SERIAL NO. : I.570147/N/A[LA-0013/LA-0013/A]  
DATE OF CALIBRATION : 10 April 2025

#### ENVIRONMENT CONDITIONS :

Temperature :  $(23 \pm 2) ^\circ\text{C}$  Relative Humidity :  $(55 \pm 10) \% \text{ RH}$

#### PROCEDURE USED :

This instrument was calibrated under procedure No. CLC-CPTH-06 based on ASTM E 220-86 as calibration guidelines.

The calibration was performed by using Calibration Bath, Precision Thermometer and IPRT which maintained by the Calibration Laboratory Co., Ltd.

#### REFERENCE STANDARD USED :

1. Calibration Bath, Kambic Model OB-22/2 ULT, OB-22/2 S/N. I7115653, I7115654.
2. Precision Thermometer, ASL Model F250 S/N. 1334023800.
3. IPRT, Wika, ASL Model CTP5000-450-D, T100-250-ID S/N. PO00036374-1-10-12, PO106346-1-18.

#### TRACEABILITY :

1. The measurements are traceable to International System of Units (SI), through Calibration Laboratory Co., Ltd. Certificate No. Q24120999, Q24112862. Due Date 26 November 2025, 12 November 2025.
2. The measurements are traceable to International System of Units (SI), through Thailand Institute of Scientific and Technological Research (TISTR). Certificate No. PSL-T 1042/67, Due Date 16 October 2025.
3. The measurements are traceable to International System of Units (SI), through National Institute of Metrology (Thailand). Certificate No. TT-0147-24, TT-0110-24. Due Date 28 October 2025, 06 August 2025.

#### UNCERTAINTY :

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor  $k = 2.00$  which for a normal distribution corresponds to a coverage probability of approximately 95 %. It has been evaluated according to the "Evaluation of the Uncertainty of Measurement in Calibration (EA-4/02 M:2022)"

Certificate No. Q25041416  
F3-011-05/12-23

page 2 of 3



@clcalibration



Accredited  
ISO/IEC 17025

**CONDITION OF CALIBRATION ITEM : RECEIVED IN GOOD OPERATIONAL CONDITION**

**MEASUREMENT RESULTS : ( X ) without adjustment ( ) adjustment**

The DUC Reading were recorded and the means value were reported of five times measurement in the table below.

**CALIBRATION DATA**

**CORRECTION OF TEMPERATURE : T1**

Immersion depth (mm)	Actual Temperature ( °C )	DUC Reading ( °C )	Correction ( °C )	Uncertainty $\pm$ ( °C )
200	4.00	4.0	0.00	0.52
	20.02	20.1	-0.08	
	95.02	96.1	-1.08	
	104.02	105.1	-1.08	
	180.00	181.6	-1.60	

Technical Note. Type of sensor : Thermocouple Type K.

Note. The Scope of Accredited ANAB Certificate No. ACDM-2814 Version 015 Page 57 of 68

This report is valid for the above stated instrument/s only.

### End of Certificate ###

Certificate No. Q25041416

F3-011-05/12-23

page 3 of 3



@clcalibration



Accredited  
ISO/IEC 17025

**CERTIFICATE OF CALIBRATION**

**FOR**

NOMENCLATURE : DIGITAL THERMOHYGRO METER  
MANUFACTURER : DIGICON  
MODEL / TYPE : TH-02A  
SERIAL NO. : 1919E0284991[DTH-01]  
CLID. NO. : 232100200  
JOB CONTROL NO. : 250408041414  
CALIBRATION SERVICE : ☒ IN-LABORATORY ☐ ON-SITE

CUSTOMER : ENVIRONMENTAL MEASUREMENTS CO., LTD.

5/45 BAAN KLANG KRUNG BIZ TOWN, SOI SRINAGARINDRA 46/1 (PRAMOTE),  
NONG BON SUB-DISTRICT, PRAWET DISTRICT, BANGKOK 10250

DATE OF RECEIVED : 08 April 2025

DATE OF ISSUED : 11 April 2025

The report of calibration shall not be reproduced except in full without approval of the Calibration Laboratory Co., Ltd.

Calibrated By :



Approved By :



Authorized Signatory

11 April 2025

This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to the

International System of Units ( SI )

Certificate No. Q25041414

F3-011-05/12-23

page 1 of 3



@clcalibration



# CALIBRATION LABORATORY Co., LTD.

2/10-11, 14, 55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230  
Tel. 02-578-0353-4 Fax: 02-578-2672 www.ccl-lab.com E-mail: sale@ccl-lab.com



ANAB  
ACCREDITED  
CALIBRATION AND  
DIMENSIONAL MEASUREMENT  
ACDM-2814

## REPORT OF CALIBRATION

### FOR

NOMENCLATURE : DIGITAL THERMOHYGRO METER  
MANUFACTURER : DIGICON  
MODEL / TYPE : TH-02A  
SERIAL NO. : 1919E0284991[DTH-01]  
DATE OF CALIBRATION : 10 April 2025

#### ENVIRONMENT CONDITIONS :

Temperature :  $(23 \pm 2) ^\circ\text{C}$  Relative Humidity :  $(55 \pm 10) \% \text{RH}$

#### PROCEDURE USED :

This instrument was calibrated under procedure No. CLC-CPTH-11. The calibration was performed by using Chilled Mirror Hygrometer which maintained by the Calibration Laboratory Co., Ltd.

#### REFERENCE STANDARD USED :

Chilled Mirror Hygrometer, Edgetech Model Dew Master S/N. 44602.  
Temperature & Humidity Chamber, PGC Model 9141-5116 S/N. 1304261.

#### TRACEABILITY :

The measurements are traceable to International System of Units (SI), through Thunder Scientific Corporation.  
Certificate No. 22724, Due Date 03 October 2025.

#### UNCERTAINTY :

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor  $k = 2.00$  which for a normal distribution corresponds to a coverage probability of approximately 95 %. It has been evaluated according to the "Evaluation of the Uncertainty of Measurement in Calibration (EA-4/02 M:2022)"

Certificate No. Q25041414

F3-011-05/12-23



page 2 of 3



# CALIBRATION LABORATORY Co., LTD.

2/10-11, 14, 55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230  
Tel. 02-578-0353-4 Fax: 02-578-2672 www.ccl-lab.com E-mail: sale@ccl-lab.com



ANAB  
ACCREDITED  
CALIBRATION AND  
DIMENSIONAL MEASUREMENT  
ACDM-2814

## CONDITION OF CALIBRATION ITEM : RECEIVED IN GOOD OPERATIONAL CONDITION

### MEASUREMENT RESULTS : ( X ) without adjustment ( ) adjustment

The table in the following gives the calibration results and associated measurement uncertainties of the measuring digital thermohygrometer.

#### CALIBRATION DATA

##### 1. CORRECTION OF TEMPERATURE

Test point ( $^{\circ}\text{C}$ )	Actual Temperature ( $^{\circ}\text{C}$ )	DUC Reading ( $^{\circ}\text{C}$ )	Correction ( $^{\circ}\text{C}$ )	Uncertainty $\pm$ ( $^{\circ}\text{C}$ )
20.0	20.00	19.6	+0.40	0.27
25.0	25.00	24.5	+0.50	
30.0	30.00	29.5	+0.50	

##### 2. CORRECTION OF HUMIDITY

STD Temperature ( $^{\circ}\text{C}$ )	STD Reading (%RH)	DUC Reading (%RH)	Correction (%RH)	Uncertainty $\pm$ (%RH)
25	40.0	30	+10.0	0.8
25	60.0	50	+10.0	0.8

Note: The Scope of Accredited ANAB Certificate No. ACDM-2814 Version 015 Page 60 of 68

This report is valid for the above stated instrument/s only.

### End of Certificate ###

Certificate No. Q25041414

F3-011-05/12-23





## CERTIFICATE OF CALIBRATION

### FOR

NOMENCLATURE : DIGITAL THERMOHYGRO METER  
MANUFACTURER : DIGICON  
MODEL / TYPE : TH-02A  
SERIAL NO. : 1919E0284980[DTH-02]  
CLID. NO. : 232100201  
JOB CONTROL NO. : 250408041415  
CALIBRATION SERVICE : ☒ IN-LABORATORY ☐ ON-SITE

CUSTOMER : ENVIRONMENTAL MEASUREMENTS CO., LTD.


5/45 BAAN KLANG KRUNG BIZ TOWN, SOI SRINAGARINDRA 46/1 (PRAMOTE),  
NONG BON SUB-DISTRICT, PRAWET DISTRICT, BANGKOK 10250

DATE OF RECEIVED : 08 April 2025

DATE OF ISSUED : 11 April 2025

The report of calibration shall not be reproduced except in full without approval of the Calibration Laboratory Co., Ltd.

Calibrated By :



Approved By :

Authorized Signatory

11 April 2025

This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to the International System of Units (SI)

Certificate No. Q25041415

F3-011-05/12-23

page 1 of 3



@clcalibration



## REPORT OF CALIBRATION

### FOR

NOMENCLATURE : DIGITAL THERMOHYGRO METER  
MANUFACTURER : DIGICON  
MODEL / TYPE : TH-02A  
SERIAL NO. : 1919E0284980[DTH-02]  
DATE OF CALIBRATION : 10 April 2025

#### ENVIRONMENT CONDITIONS :

Temperature :  $(23 \pm 2) ^\circ\text{C}$  Relative Humidity :  $(55 \pm 10) \% \text{RH}$

#### PROCEDURE USED :

This instrument was calibrated under procedure No. CLC-CPTH-11. The calibration was performed by using Chilled Mirror Hygrometer which maintained by the Calibration Laboratory Co., Ltd.

#### REFERENCE STANDARD USED :

Chilled Mirror Hygrometer, Edgetech Model Dew Master S/N. 44602.  
Temperature & Humidity Chamber, PGC Model 9141-5116 S/N. 1304261.

#### TRACEABILITY :

The measurements are traceable to International System of Units (SI), through Thunder Scientific Corporation.  
Certificate No. 22724, Due Date 03 October 2025.

#### UNCERTAINTY :

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor  $k = 2.00$  which for a normal distribution corresponds to a coverage probability of approximately 95 %.  
It has been evaluated according to the "Evaluation of the Uncertainty of Measurement in Calibration (EA-4/02 M:2022)"

Certificate No. Q25041415

F3-011-05/12-23

page 2 of 3



@clcalibration



CONDITION OF CALIBRATION ITEM : RECEIVED IN GOOD OPERATIONAL CONDITION  
MEASUREMENT RESULTS : ( X ) without adjustment ( ) adjustment

The table in the following gives the calibration results and associated measurement uncertainties of the measuring digital thermohygro meter.

CALIBRATION DATA

1. CORRECTION OF TEMPERATURE

Test point ( ° C )	Actual Temperature ( ° C )	DUC Reading ( ° C )	Correction ( ° C )	Uncertainty ± ( ° C )
20.0	20.00	19.7	+0.30	0.27
25.0	25.00	24.6	+0.40	
30.0	30.00	29.5	+0.50	

2. CORRECTION OF HUMIDITY

STD Temperature ( ° C )	STD Reading ( %RH )	DUC Reading ( %RH )	Correction ( %RH )	Uncertainty ± ( %RH )
25	40.0	33	+7.0	0.8
25	60.0	53	+7.0	0.8

Note. The Scope of Accredited ANAB Certificate No. ACDM-2814 Version 01.5 Page 60 of 68

This report is valid for the above stated instrument/s only.

### End of Certificate ###



CERTIFICATE OF CALIBRATION

FOR

NOMENCLATURE : WATER BATH  
MANUFACTURER : M-LAB  
MODEL / TYPE : WBN 15  
SERIAL NO. : 0335[LA-007]  
CLID. NO. : 332300657  
JOB CONTROL NO. : 250215018258  
CALIBRATION SERVICE : ☐ IN-LABORATORY ☒ ON-SITE

CUSTOMER : ENVIRONMENTAL MEASUREMENTS CO., LTD.


5/45 BAAN KIANG KRUNG BIZ TOWN, SOI SRINAGARINDRA 46/1 (PRAMOTE),  
NONG BON SUB-DISTRICT, PRAWET DISTRICT, BANGKOK 10250

DATE OF RECEIVED : 15 February 2025

DATE OF ISSUED : 04 March 2025

The report of calibration shall not be reproduced except in full without approval of the Calibration Laboratory Co., Ltd.

Calibrated By :



Approved By :



Authorized Signatory  
04 March 2025

This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to the International System of Units ( SI )







**CALIBRATION LABORATORY Co., LTD.**  
2/10-11,14, 55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230  
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



## REPORT OF CALIBRATION

### FOR

NOMENCLATURE : WATER BATH  
MANUFACTURER : M-LAB  
MODEL / TYPE : WBN 15  
SERIAL NO. : 0335[LA-007]  
LOCATION SITE : LABORATORY - HOT ZONE  
DATE OF CALIBRATION : 27 February 2025

#### ENVIRONMENT CONDITIONS :

Temperature : 24 °C to 25 °C Relative Humidity : 49% to 51%

#### PROCEDURE USED :

This instrument was calibrated under procedure No. W1-305-135 based on ASTM E 715-80:2016 as calibration guidelines.  
The calibration was performed by using Hydra Data Logger which maintained by the Calibration Laboratory Co., Ltd.

#### REFERENCE STANDARD USED :

Hydra Data Logger, Fluke Model 2620 S/N. 5592550.

#### TRACEABILITY :

The measurements are traceable to International System of Units (SI), through Calibration Laboratory Co., Ltd.  
Certificate No. Q24120965, Due Date 13 May 2025.

#### UNCERTAINTY :

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor  $k = 2.00$  which for a normal distribution corresponds to a coverage probability of approximately 95 %.  
It has been evaluated according to the "Evaluation of the Uncertainty of Measurement in Calibration (EA-4/02 M:2022)"

Certificate No. Q25018258

F3-011-05/12-23

page 2 of 4



@clcalibration



**CALIBRATION LABORATORY Co., LTD.**  
2/10-11,14, 55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230  
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



## CONDITION OF CALIBRATION ITEM : RECEIVED IN GOOD OPERATIONAL CONDITION

### MEASUREMENT RESULTS : ( X ) without adjustment ( ) adjustment

The table in the following gives the calibration results and associated measurement uncertainties of the measuring water bath.

#### CALIBRATION DATA

##### 1. WATER BATH PERFORMANCE

Test Point ( °C )	DUC Reading ( °C )	Uniformity ( °C )	Stability ( °C )
85.0	85.0	0.40	0.28

Certificate No. Q25018258

F3-011-05/12-23

page 3 of 4



@clcalibration




CALIBRATION DATA

2. TEMPERATURE DISTRIBUTION

Test Point ( ° C )	DUC Reading ( ° C )	STD Reading ( ° C )					Uncertainty ± ( ° C )
		Probe No. 1	Probe No. 2	Probe No. 3	Probe No. 4	Probe No. 5	
85.0	85.0	85.15	84.79	84.96	84.89	85.06	0.58

Technical Note : W = 35 cm, D = 30 cm, H = 15 cm.

The Scope of Accredited TISI Certificate No. 23-LB0092 Issue 02 Page 128 of 138

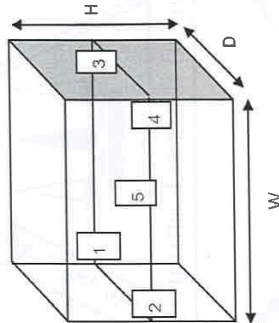

This report is valid for the above stated instrument/s only.

### End of Certificate ###

Certificate No. Q25018258

F3-011-05/12-23

page 4 of 4



@cccalibration



CERTIFICATE OF CALIBRATION

FOR

NOMENCLATURE : WATER BATH  
MANUFACTURER : MEMMERT  
MODEL / TYPE : WNB14  
SERIAL NO. : L418.0758[LA-004]  
CLID. NO. : 332100157  
JOB CONTROL NO. : 250215018257  
CALIBRATION SERVICE : ☐ IN-LABORATORY ☒ ON-SITE

CUSTOMER : ENVIRONMENTAL MEASUREMENTS CO., LTD.

5/45 BAAN KLANG KRUNG BIZ TOWN, SOI SRINAGARINDRA 46/1 (PRAMOTE),  
NONG BON SUB-DISTRICT, PRAWET DISTRICT, BANGKOK 10250

DATE OF RECEIVED : 15 February 2025

DATE OF ISSUED : 04 March 2025

The report of calibration shall not be reproduced except in full without approval of the Calibration Laboratory Co., Ltd.

Calibrated By :



Approved By :

Authorized Signatory

04 March 2025

This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to the International System of Units (SI)

Certificate No. Q25018257

F3-011-05/12-23

page 1 of 4



@cccalibration



**CALIBRATION LABORATORY Co., LTD.**  
2/10-11,14, 55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230  
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cah-laboratory.com E-mail:sale@cal-laboratory.com



## REPORT OF CALIBRATION

### FOR

NOMENCLATURE : WATER BATH  
MANUFACTURER : MEMMERT  
MODEL / TYPE : WNB14  
SERIAL NO. : L418.0758[LA-004]  
LOCATION SITE : LABORATORY - HOT ZONE  
DATE OF CALIBRATION : 27 February 2025

#### ENVIRONMENT CONDITIONS :

Temperature : 24 °C to 25 °C

Relative Humidity : 49% to 51%

#### PROCEDURE USED :

This instrument was calibrated under procedure No. W1-305-135 based on ASTM E 715-80:2016 as calibration guidelines.  
The calibration was performed by using Hydra Data Logger which maintained by the Calibration Laboratory Co., Ltd.

#### REFERENCE STANDARD USED :

Hydra Data Logger, Fluke Model 2620 S/N. 5592550.

#### TRACEABILITY :

The measurements are traceable to International System of Units (SI), through Calibration Laboratory Co., Ltd.  
Certificate No. Q24120965, Due Date 13 May 2025.

#### UNCERTAINTY :

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor  $k = 2.00$  which for a normal distribution corresponds to a coverage probability of approximately 95 %.  
It has been evaluated according to the "Evaluation of the Uncertainty of Measurement in Calibration (EA-4/02 M:2022)"

Certificate No. Q25018257

F3-011-05/12-23

page 2 of 4



@clcalibration



**CALIBRATION LABORATORY Co., LTD.**  
2/10-11,14, 55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230  
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cah-laboratory.com E-mail:sale@cal-laboratory.com



## CONDITION OF CALIBRATION ITEM : RECEIVED IN GOOD OPERATIONAL CONDITION

### MEASUREMENT RESULTS : ( X ) without adjustment ( ) adjustment

The table in the following gives the calibration results and associated measurement uncertainties of the measuring water bath.

#### CALIBRATION DATA

##### 1. WATER BATH PERFORMANCE

Test Point ( °C )	DUC Reading ( °C )	Uniformity ( °C )	Stability ( °C )
95.0	95.0	0.39	0.17

Certificate No. Q25018257

F3-011-05/12-23

page 3 of 4



@clcalibration



Accredited  
ISO/IEC 17025

## CALIBRATION LABORATORY CO., LTD.

2/10-11, 14, 55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230  
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cclaboratory.com E-mail: sale@cclaboratory.com



NSC-TISI-TIS 17025  
CALIBRATION 0059  
CLC




### CALIBRATION DATA

#### 2. TEMPERATURE DISTRIBUTION

Test Point ( ° C )	DUC Reading ( ° C )	STD Reading ( ° C )					Uncertainty ± ( ° C )
		Probe No. 1	Probe No. 2	Probe No. 3	Probe No. 4	Probe No. 5	
95.0	95.0	96.45	96.30	96.22	96.04	96.26	0.51

Technical Note : W = 35 cm, D = 29 cm, H = 14 cm.

The Scope of Accredited TISI Certificate No. 23-LB0092 Issue 02 Page 128 of 138

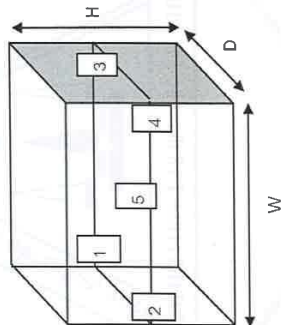

This report is valid for the above stated instrument/s only.

### End of Certificate ###

Certificate No. Q25018257

F3-011-05/12-23

page 4 of 4



@cclibration