

ภาคผนวก ฉ
เอกสารสอบเทียบเครื่องมือ

List of Instrument Certificates for Environmental Quality Analysis

No.	Instrument/Equipment	Parameter	Manufacturer	Model/Serial No.	Calibrator	Certification No.	Date of Calibration	Due date of Calibration*
1	Atomic Absorption Spectrometer	CADMIUM CHROMIUM TRIVALENT COPPER LEAD MANGANESE MERCURY NICKEL ZINC	Agilent Technologies	AA240FS / MY13160001	Agilent Technologies (Thailand) Co.,Ltd.	Preventive Maintenance Checklist	24/1/2024	23/1/2025
			Agilent Technologies	AA240FS / MY13160001	Agilent Technologies (Thailand) Co.,Ltd.	Preventive Maintenance Checklist	30/1/2025	29/1/2026
2	Atomic Absorption Spectrometer	ARSENIC SELENIUM	Perkin Elmer	PinAAcle 900F / PFB20031902	Perkin Elmer Co.,Ltd.	WO-02787590	14/5/2024	13/5/2025
			Perkin Elmer	PinAAcle 900F / PFB20031902	Perkin Elmer Co.,Ltd.	Preventive Maintenance Report	29/4/2025	28/4/2026
3	Analytical Balance	FAT OIL AND GREASE	Mettler Toledo	AB204-S/FACT / 1129361010	Technology Promotion Association (Thailand-Japan)	24MM292	11/5/2024	10/5/2025
			Mettler Toledo	AB204-S/FACT / 1129361010	United Analyst and Engineering Consultant Co., Ltd.	250422 1 BL002 25	23/4/2025	22/4/2026
4	Analytical Balance	TOTAL DISSOLVED SOLIDS	Mettler Toledo	XSR205DU / C210685394	National Food Institute,Ministry of Industry, Thailand	2402283-002-01	2/4/2024	1/4/2025
			Mettler Toledo	XSR205DU / C210685394	National Food Institute,Ministry of Industry, Thailand	2502226-002-01	20/3/2025	19/3/2026

List of Instrument Certificates for Environmental Quality Analysis

No.	Instrument/Equipment	Parameter	Manufacturer	Model/Serial No.	Calibrator	Certification No.	Date of Calibration	Due date of Calibration*
5	Analytical Balance	TOTAL DISSOLVED SOLIDS TOTAL SUSPENDED SOLIDS	Mettler Toledo	XSR205DU / C009071872	National Food Institute,Ministry of Industry, Thailand	2402283-001-01	2/4/2024	1/4/2025
			Mettler Toledo	XSR205DU / C009071872	National Food Institute,Ministry of Industry, Thailand	2502226-001-01	20/3/2025	19/3/2026
6	BOD Incubator	BIOCHEMICAL OXYGEN DEMAND	ARCO	UC4-1320 / 1021	Technology Promotion Association (Thailand-Japan)	24TM1113	11/7/2024	16/7/2025
7	BOD Incubator	BIOCHEMICAL OXYGEN DEMAND	ARCO	UC4-1320 / 1021	Technology Promotion Association (Thailand-Japan)	24TM1114	11/7/2024	10/7/2025
8	BOD Incubator	BIOCHEMICAL OXYGEN DEMAND	ARCO	UR-1320 / -	Technology Promotion Association (Thailand-Japan)	24TM588	1/4/2024	31/3/2025
9	Continuous Flow Analyzer(CFA)	CYANIDE	Skalar Analytical B.V., the Netherlands	San++5000-02 / 182688	DKSH (Thailand) Ltd.	Service Report/Test Report WO-00018067	20/2/2024	19/2/2025
			Skalar Analytical B.V., the Netherlands	San++5000-02 / 182688	DKSH (Thailand) Ltd.	WO-00074079	23/5/2025	22/5/2026
10	DO Meter	DO	Horiba	LAQUA-DO210 / HE9M0013	Technology Promotion Association (Thailand-Japan)	24TW271	25/12/2024	24/12/2025
11	DO Meter	DO	Horiba	LAQUA-DO210 / HE2L0016	Technology Promotion Association (Thailand-Japan)	24TW57	14/3/2024	12/3/2025
12	DO Meter	DO	Horiba	LAQUA-DO210 / HE2L0040	Technology Promotion Association (Thailand-Japan)	25TW36	26/2/2025	25/2/2026
13	DO Meter	DO	Horiba	LAQUA-DO210 / HE1L0034	Technology Promotion Association (Thailand-Japan)	25TW25	5/2/2025	3/2/2026
14	DO METER	DO	Horiba	LAQUA-DO210 / HE0H0008	Technology Promotion Association (Thailand-Japan)	25TW27	10/2/2025	9/2/2026

List of Instrument Certificates for Environmental Quality Analysis

No.	Instrument/Equipment	Parameter	Manufacturer	Model/Serial No.	Calibrator	Certification No.	Date of Calibration	Due date of Calibration*
15	DO Meter	BIOCHEMICAL OXYGEN DEMAND	YSI	5100 / 11B 101863	Technology Promotion Association (Thailand-Japan)	24TW39	21/2/2024	20/2/2025
			YSI	5100 / 11B 101863	Technology Promotion Association (Thailand-Japan)	25TW29	18/2/2025	16/2/2026
16	DO Meter	DO	YSI Environmental	Pro 20i / 18F103884	Technology Promotion Association (Thailand-Japan)	24TW179	27/8/2024	25/7/2025
17	Digestion Units	TOTAL KJELDAHL NITROGEN	Foss Tecator	2520 Auto / 91794469			27/1/2025	26/1/2026

List of Instrument Certificates for Environmental Quality Analysis

No.	Instrument/Equipment	Parameter	Manufacturer	Model/Serial No.	Calibrator	Certification No.	Date of Calibration	Due date of Calibration*
18	Gas Chromatography	a-BHC ALDRIN b-BHC BIFENTHRIN CHLORDANE cis-CHLORDANE CYFLUTHRIN CYPERMETHRIN d-BHC DDD DDE DDT DELTAMETHRIN DIELDRIN ENDOSULFAN I ENDOSULFAN II ENDOSULFAN SULFATE ENDRIN ENDRIN ALDEHYDE FENVALERATE g-BHC HEPTACHLOR HEPTACHLOR EPOXIDE LAMBDA-CYHALOTHRIN METHOXYCHLOR op-DDD op-DDE op-DDT PERMETHRIN pp-DDD	Agilent	GC 7890A / CN11021007	Agilent Technologies (Thailand) Co.,Ltd.	Certificate of System Qualification GC-OQ	21/2/2024	19/2/2025

List of Instrument Certificates for Environmental Quality Analysis

No.	Instrument/Equipment	Parameter	Manufacturer	Model/Serial No.	Calibrator	Certification No.	Date of Calibration	Due date of Calibration*
		pp-DDE pp-DDT trans-CHLORDANE						
			Agilent	GC 7890A / CN11021007	Agilent Technologies (Thailand) Co.,Ltd.	Certificate of System Qualification GC-OQ	18/2/2025	17/2/2026
19	Gas Chromatography	CHOLRPYRIFOS DIMETHOATE EPN ETHOPROPHOS MALATHION METHAMIDOPHOS METHIDATHION METHYL PARATHION MEVINPHOS MONOCROTOPHOS PHOSALONE PROFENOFOS TRIAZOPHOS	Agilent	7890B GC / CN13113001	Agilent Technologies (Thailand) Co.,Ltd.	Certificate of System Qualification GC-OQ	1/4/2025	31/3/2026
20	Heating Block	CHEMICAL OXYGEN DEMAND	Hanna Instruments Italia Srl.	HI 839800-02 / H 018500 I	Hanna Instruments (Thailand) Ltd.	HIT-2412-0389	18/3/2024	17/3/2025
			Hanna Instruments Italia Srl.	HI 839800-02 / H 018500 I	Hanna Instruments (Thailand) Ltd.	HIT-2510-0375	7/3/2025	6/3/2026
21	Heating Block	CHEMICAL OXYGEN DEMAND	Hanna Instruments Inc.(Romania)	HI839800-02 / 4500052101	Hanna Instruments (Thailand) Ltd.	HIT-2427-0942	1/7/2024	30/6/2025
22	Mercury Analyzer	TOTAL MERCURY	NIC. Japan	RA-4500 / 17780278	Coax Group Corporation Ltd.	Preventive Maintenance Report	9/7/2024	8/7/2025
23	Hot Air Oven	TOTAL DISSOLVED SOLIDS TOTAL SUSPENDED SOLIDS	Memmert	UF55 / B212.0411	Technology Promotion Association (Thailand-Japan)	24TM589	1/4/2024	31/3/2025

List of Instrument Certificates for Environmental Quality Analysis

No.	Instrument/Equipment	Parameter	Manufacturer	Model/Serial No.	Calibrator	Certification No.	Date of Calibration	Due date of Calibration*
24	Cooled Incubator	TOTAL COLIFORM BACTERIA FECAL COLIFORM BACTERIA	Binder	KB400 / WTB20200000015535	Technology Promotion Association (Thailand-Japan)	24TM647	1/4/2024	31/3/2025
25	Incubator	TOTAL COLIFORM BACTERIA FECAL COLIFORM BACTERIA	Binder	KB400 / 20220000022479	Technology Promotion Association (THAILAND-JAPAN)	24TM938	9/7/2024	8/7/2025
26	Incubator	TOTAL COLIFORM BACTERIA FECAL COLIFORM BACTERIA	Binder	KB400 / 20220000000391	Technology Promotion Association (Thailand-Japan)	24TM884	7/6/2024	6/6/2025
27	Inductively Coupled Plasma- Optical Emission Spectrometer(ICP-OES)	BARIUM CADMIUM	Agilent Technologies, USA	5110 VDV(G8015AA) / MY8030001	Agilent Technologies (Thailand) Co.,Ltd.	Preventive Maintenance Checklist	4/11/2024	3/11/2025
28	Kjeltec Distillation Unit	TOTAL KJELDAHL NITROGEN	FOSS	KT9 / 91905393	FOSS South East Asia	12875	5/7/2024	4/7/2025
29	pH Meter	pH	Horiba	LAQUA-PH210 / HA9M0047	technology promotion association (thailand-japan	24CH400	3/4/2024	1/4/2025
			Horiba	LAQUA-PH210 / HA9M0047	technology promotion association (thailand-japan	25CH354	20/3/2025	18/3/2026
30	pH Meter	pH	Horiba	LAQUA-PH210 / HA1L0035	technology promotion association (thailand-japan	25CH262	28/2/2025	27/2/2026
31	pH Meter	pH	Horiba	LAQUA-PH210 / HA1M0043	technology promotion association (thailand-japan	25CH263	28/2/2025	27/2/2026
32	pH Meter	pH	Horiba	LAQUA-PH210 / HA0E0006	technology promotion association (thailand-japan	24CH726	19/6/2024	17/6/2025
33	pH Meter	pH	Horiba	LAQUA-PH210 / HA0C0025	technology promotion association (thailand-japan	24CH319	14/3/2024	13/3/2025
34	pH Meter	pH	YSI Environmental	pH 100A / JC03354	Technology Promotion Association (Thailand-Japan)	24CH1379	5/11/2024	6/11/2025
35	pH Meter	pH	YSI Environmental	pH 100A / JC02729		24CH1070	27/8/2024	25/7/2025

List of Instrument Certificates for Environmental Quality Analysis

No.	Instrument/Equipment	Parameter	Manufacturer	Model/Serial No.	Calibrator	Certification No.	Date of Calibration	Due date of Calibration*
36	Spectrophotometer	CHEMICAL OXYGEN DEMAND CHROMIUM HEXAVALENT COLOUR (pH 7.0) COLOUR (pH Sample)	Agilent	Cary 60 G6860A / MY15410009	DQE Services Co.,Ltd.	SP24-018	7/5/2024	6/5/2025
			Agilent	Cary 60 G6860A / MY15410009	DQE Services Co.,Ltd.	SP25-019	26/5/2025	25/5/2026
37	UV-VIS Spectrophotometer	FORMALDEHYDE PHOSPHATE	Hitachi	U-1900 / 2021-064	DQE Services Co.,Ltd.	SP24-008	16/1/2024	15/1/2025
38	UV-VIS Spectrophotometer	NITRATE NITROGEN TOTAL PHOSPHORUS	Hitachi	U-2900 / 21E22-009	DQE Services Co.,Ltd.	SP25-001	3/1/2025	2/1/2026
39	UV/VIS Spectrophotometer	AMMONIA-NITROGEN CHEMICAL OXYGEN DEMAND FORMALDEHYDE PHENOLS	Hitachi	U-5100 / 23A4-008	DQE Services Co.,Ltd.	SP24-028	11/9/2024	9/9/2025

Due Date of Calibration* : Based on the annual calibration plan. At least 1 time per year.

List of Instrument Certificates for Environmental Quality Analysis

No.	Instrument/Equipment	Parameter	Manufacturer	Model/Serial No.	Calibrator	Certification No.	Date of Calibration	Due date of Calibration*
1	Analytical Balance	PARTICULATE MATTER (PM10) TOTAL SUSPENDED PARTICULATE	Mettler Toledo	MS204TS/00 / C252436235	National Food Institute, Ministry of Industry, Thailand	2502228-003-01	19/3/2025	18/3/2026

Due Date of Calibration* : Based on the annual calibration plan. At least 1 time per year.

Agilent 55 240 280 Series Atomic Absorption Spectroscopy Systems

Preventive Maintenance Checklist

Agilent Preventive Maintenance provides factory recommended service for your analytical systems to assure reliable operation and the accuracy of your results.

Delivered by highly trained and certified service engineers using genuine Agilent parts and supplies, Agilent Preventive Maintenance provides everything you need to reduce unplanned downtime and keep your systems operating at their peak. This checklist will be completed at the end of the service and provided to you as a record of the installation.

Note: While non-current production AA instrument and/or accessory models are not covered specifically in this document it can be used as a basic reference.

For more information about Agilent Technologies services please visit our web site using the following URL: <http://www.agilent.com/en-us/services>

Introduction

Customer Information

- Customers should provide all necessary operating supplies upon request of the engineer.
- A customer representative should be available to the engineer while performing the preventive maintenance procedures.
- Any parts, not included in the Parts Lists section of this document, are not part of the recommended Preventive Maintenance service, nor are they included in the price of this service.
- If a system requires the use of extra or special procedures and/or parts for the maintenance service, then these must be ordered separately and charged as a repair, which may incur additional costs.

Revision: 10.00, Issued: November 2021

© Agilent Technologies, Inc. 2021



Important Customer Web Links

- For more information about Agilent Technologies services, please visit our website using the following URL: <http://www.agilent.com/en-us/products/crosslab-instrument-services/service-repair>
- To access Agilent University, visit <http://www.agilent.com/crosslab/university/> to learn about training options, which include online, classroom and onsite delivery. A training specialist can work directly with you to help determine your best options.
- A useful Agilent Resource Center web page is available, which includes short videos on maintenance, quick lists of consumables for new instruments, and other valuable information. Check out the Resource Page here: <https://www.agilent.com/en-us/agilentresources>
- Need technical support, FAQs, supplies? – visit our Support Home page at <http://www.agilent.com/search/support>
- Get answers. Share insights. Build connections: Join the Agilent Community at <https://community.agilent.com/welcome>

Service Engineer's Responsibilities

- Contact the customer and ensure that all necessary supplies are available before the preventive maintenance visit.
 - Confirm the ability of the instrument to deliver continued safe operation as established via the Agilent AA safe operation flow chart. (Refer directly to the AA 55/240/280 Preventive Maintenance Scope of Work to make this decision.)
 - Only select those pages that relate to the system or module being serviced.
 - Complete empty fields with the relevant information.
 - Complete the relevant checkboxes in the checklist using either a "X" or tick mark "✓".
 - Check "Section not applicable" check boxes to indicate services/tasks not delivered, as appropriate.
 - Complete the Preventive Maintenance service in the order of the tasks listed.
 - Complete the Service Review section together with the customer.
 - Complete the fields for page numbers at the foot of each selected page
 - Complete the total number of pages field in the Service Completion section
 - Ask the customer to sign the Service Completion section including the customer's and your signature.
- This information is subject to change without notice.

Revision: 10.00, Issued: November 2021

© Agilent Technologies, Inc. 2021



Instrument Maintenance

System Information

- ☐ Check this box if an instrument configuration report is attached instead of completing the table.

Instrument System Name and ID	240 FS AAS
Instrument System Site and Location	United Analyst and Engineering Consultant

List System Component Product Numbers	List the Serial Numbers of each Component
1. G 9432 A	M 13160001
2.	
3.	
4.	
5.	
6.	
7.	
8.	
9.	

Preparation, Safe operation and Initial performance checks

Revision: 10.00, Issued: November 2021

© Agilent Technologies, Inc. 2021



- ☐ Agilent AA safe operation flow chart inspections (to determine if the PM can be performed).

NOTE: If by following the flow chart the instrument is deemed to be unsafe for continued use you MUST NOT continue PM work. Inform the customer immediately of the Agilent recommendation that use of the instrument be discontinued.

- ☒ Discuss any specific issues with the customer before starting.
- ☐ For HF application systems, if standard sample introduction system was not installed, ask the customer to install it. **NA**
- ☒ Review the instrument logbook for recorded problems and comments.
- ☒ Save instrument control settings before starting the procedure.
- ☒ Perform a general inspection of the system for cleanliness.
- ☒ Check for proper installation of parts, assemblies, sensors etc.
- ☒ Check system for required installation of components, settings as defined by current Service Notes
- ☒ Check for required firmware updates and verify with customers if they would like them installed.
- ☒ Use SVD to perform a Full Wavelength Scan for Cu HCL - "As found test_1"
- ☒ Perform a Basic Cu ABS test - "As found test_2"
- ☒ Print the Details page or screen captures of the test results and attach to the end of this checklist.

Revision: 10.00, Issued: November 2021

© Agilent Technologies, Inc. 2021



Preventive Maintenance Procedures

FLAME SYSTEM section

☐ Section not applicable

Electronic components

- ☒ Review and confirm instrument configuration data in SVD
- ☒ Confirm power supply voltages using the *SVD Power Supply diagnostic*.
- ☒ For Dual Beam Instruments - Confirm RBC frequency using the *SVD RBC frequency diagnostic*.

Mechanical components

- ☒ Check the burner adjuster controls for complete and free movement. If the burner adjuster needs lubrication, use Molykote 321 or mineral-based molybdenum disulphide grease.
- ☒ Run SVD tests to exercise all motor drives over the full range of their travel:
 - ☒ Monochromator drive
 - ☒ Slit drive
 - ☒ Lamp selector
 - ☐ ABA

Optics components

- ☒ Check that external optical surfaces are clean – Clean or replace as required.
- ☒ Use SVD and perform *Mono Wavelength Correction*.
- ☒ Use SVD and perform *Slit Calibration*.
- ☒ Use SVD and perform *Grating Squareness Diagnostic*.
- ☒ Use SVD and perform *Zero Order Offset/Mono Correction*.
- ☒ Use SVD and perform *Wavelength Repeatability*.
- ☒ Physically inspect selected HC lamps (customer to supply per their choice) and measure the % Gain for each lamp. Advise customer if lamps are showing emission degradation due to age.
- ☒ Check that the signal energy of the D2 and HC lamps track properly. Advise customer if their D2 lamp is showing emission degradation due to age.

Revision: 10.00, Issued: November 2021

© Agilent Technologies, Inc. 2021



Sample Introduction and Atomization

- ☒ Inspect the burner interlock plate to ensure that the interlock pin is secure and correct for the burner type.
- ☒ Clean the burner slot with a clean white card.
- ☒ Check the uniformity of the slot width.
- ☒ Clean the burner if required.
- ☒ Change the burner o-ring.
- ☒ Clean the nebulizer, spray chamber and liquid trap.
- ☒ Change all o-rings and seals in the nebulizer, nebulizer block and spray chamber.
- ☒ Check that the pressure relief bung releases readily.
- ☒ Change o-rings on the fuel and oxidant delivery bars.
- ☒ Leave the liquid trap EMPTY and verify the flame will not ignite in this state.
- ☒ Refill liquid trap and check that overflow drains freely into the drain/waste tube.
- ☒ Check the drain/waste tube for good drainage. It should not have tight bends, kinks or loops and the lower end must be above the liquid level in the waste vessel
- ☒ Check and clean the igniter electrode

Gas handling components and safety interlocks

- ☒ Pressure test for leaks
- ☒ Leak test gasbox internal components and connections
- ☒ Check safety interlock status and operation using the *SVD interlock monitoring diagnostic*.

Analytical performance for Flame systems

- ☒ Ignite a flame.
- ☒ Check that you can adjust the nebulizer uptake rate from 4 to 6.5 mL per minute.
- ☒ Optimize the instrument ready to perform Cu sensitivity test.
- ☒ Create a manual method to perform a Basic Cu ABS test - "Final Performance Testing"
- ☒ Run a PM completed sensitivity test for a 5 ppm copper sample and record the results in the AA PM Performance test results and measurements table.

Revision: 10.00, Issued: November 2021

© Agilent Technologies, Inc. 2021



FURNACE SYSTEM section

☒ Section not applicable

Electronic components

- ☐ Review and confirm instrument configuration data in SVD
- ☐ Confirm power supply voltages using the *SVD Power Supply diagnostic*.

Mechanical components

- ☐ Run SVD tests to exercise all motor drives over the full range of their travel:
 - ☐ Monochromator drive
 - ☐ Slit drive
 - ☐ Lamp selector

Optics components

- ☐ Check that external optical surfaces are clean – Clean or replace as required.
- ☐ Use SVD and perform *Mono Wavelength Correction*.
- ☐ Use SVD and perform *Slit Calibration*.
- ☐ Use SVD and perform *Grating Squareness Diagnostic*.
- ☐ Use SVD and perform *Zero Order Offset/Mono Correction*.
- ☐ Use SVD and perform *Wavelength Repeatability*.
- ☐ Physically inspect selected HC lamps (customer to supply per their choice) and measure the % Gain for each lamp. Advise customer if lamps are showing emission degradation due to age.

Gas handling, water system and workhead component checks

- ☐ Inspect the GTA workhead gas hoses and connections for leaks.
- ☐ Pressure test for gas leaks
- ☐ If the cooler system is accessible (stand-alone) check for correct operation and coolant/water level – this includes any temperature and pressure settings plus filter cleaning (air flow and water).
- ☐ Inspect the GTA workhead water hoses and connections for leaks.
- ☐ Check all graphite components and replace if necessary.

Revision: 10.00, Issued: November 2021

© Agilent Technologies, Inc. 2021



- ☐ Tube
- ☐ Electrodes
- ☐ Shroud

- ☐ Check and clean the end windows on the workhead.
- ☐ Check safety interlock operation.

Analytical performance for Furnace systems

- ☐ Optimize the instrument ready to perform Cu sensitivity test.
- ☐ Run the sensitivity test for a 25 ppb copper sample and record the results in the results table.

PSD autosampler accessory for Furnace systems

- ☒ Section NOT Applicable
- ☐ Check condition of the PSD capillary – replace if necessary
- ☐ Check condition and operation of PSD syringe – ensure it does not have air locks and bubbles.
- ☐ Change PSD rinse bottle o-ring.
- ☐ Check and clean the rinse vessel.
- ☐ Check the drain tube for good drainage. It should not have tight bends, kinks or loops and the lower end must be above the liquid level in the waste vessel.
- ☐ Ensure that the waste vessel is suitable for use with the furnace system.

Sample introduction pump system (SIPS) accessory

- ☒ Section NOT Applicable
- ☐ Re-torque screws securing the hubs, presser arms and pump rotors.
- ☐ Adjust each roller so that it rotates freely.
- ☐ Wipe clean the pump rotor rollers and pump bands with a dry clean cloth.
- ☐ Ensure that the presser arms and the surfaces near the pump are free from dirt and spills.
- ☐ Remove the pump module rear cover and check for the incursion of liquids and any signs of corrosion.
- ☐ Re-torque the nuts that fasten the motor mounting plates to the chassis.
- ☐ Check clips securing the diluents holder and replace if necessary.
- ☐ Disconnect, clean T-piece, and reassemble the tubing using the following steps.

Revision: 10.00, Issued: November 2021

© Agilent Technologies, Inc. 2021



- ☐ Remove the T-piece by disconnecting the pump tubes, the pump bands and all other tubing.
- ☐ Place the T-piece in an ultrasonic bath containing strong detergent 1-5% Decon 30 or similar, for approximately 5-10 minutes.
- ☐ Wash the T-piece under a tap with a strong flow of water.
- ☐ Rinse with distilled water through all of the inlets in the reverse direction to normal sample flow.
- ☐ Reassemble.

Sample preparation system (SPS 4) accessory

☒ Section NOT Applicable

The Agilent SPS 4 autosampler is designed to need minimal maintenance.

The following maintenance requirements are suggested to maintain the performance of the autosampler.

- ☐ Cleaning the spill tray, rack location mat, end frames and chassis accessories with a damp soft cloth and diluted mild detergent.
- ☐ Cleaning the autosampler cover panels with domestic window cleaner.
- ☐ Checking the X- axis and Z- axis drive belts for cracks, splits, damaged teeth, excessive fraying, color changes or degradation from fumes.
- ☐ Check the X- axis, Theta- axis and Z- axis FFC cables for cracks, incorrect positioning, damaged edge or damaged connectors.

NOTE: The autosampler requires no extra lubrication throughout its lifetime.

For further details refer to the SPS 4 service manual G8410-90050.

Sample preparation system (SPS 3) accessory

☒ Section NOT Applicable

- ☐ Check the x-axis and z-axis timing belts – Replace if there is any cracks, splits or color deterioration and belt tension.
- ☐ Check belt tensions - adjust if required
- ☐ Check the lubrication pad for single x-axis shaft. If pad is dry or customer has observed any vibration or erratic movements of the x-axis carriage, add 1 mL of Dow Corning 200 @ Fluid, 200 CS into the well.
- ☐ Check the auto-sampler ability to find tube positions - Calibrate if required.
- ☐ Clean the exterior surfaces of the accessory with soft lint free cloth. This cloth can be dampened with warm water or a mild detergent. Do not use organic solvents or abrasive cleaning agents.

Revision: 10.00, Issued: November 2021

© Agilent Technologies, Inc. 2021



Vapor generation accessory VGA (hydride generator)

☒ Section NOT Applicable

- ☐ Inspect VGA gas supply hose.
- ☐ Inspect/replace VGA pump tubing.
- ☐ Check low gas pressure interlock setting – adjust if required.
- ☐ Check precision orifice gas flow setting – adjust if required.
- ☐ Check gas regulator pressure to 46 psi (325 kPa) – adjust if required.
- ☐ Clean the exterior surfaces of the accessory with soft lint free cloth. This cloth can be dampened with warm water or a mild detergent. Do not use organic solvents or abrasive cleaning agents.

UltrAA lamp accessory (external)

☒ Section NOT Applicable

- ☐ Check the condition of the power cable.
- ☐ Clean the exterior surfaces of the accessory with soft lint free cloth. This cloth can be dampened with warm water or a mild detergent. Do not use organic solvents or abrasive cleaning agents.

Restore System

- ☐ If you have altered the customer's instrumentation during the course of PM, restore to the original status to allow the customer to conduct their normal activities (e.g., reload the customer's method.)

Guidance

If the PM service is performed prior to a qualification service, then use the qualification procedure as a guide for final instrument set up and checkout.

Revision: 10.00, Issued: November 2021

© Agilent Technologies, Inc. 2021



Signature Page

Service Review

- ☒ Attach available reports/printouts of all tests to this documentation.
- ☒ Record the Preventive Maintenance service activity in the customer's records/logbook.
- ☒ Update/reset instrument maintenance counters as appropriate.
- ☒ Affix the PM sticker to the system or instrument logbook based on the customer's request.
- ☒ Complete the Service Engineer Comments section if there are additional comments.
- ☒ Review this service, parts replaced, and test results obtained with the customer.
- ☒ If the instrument firmware was updated, record the details of the change in the Service Engineer's Comments box or if necessary, in the customer's IQ records.

Test Results

Test Description	Expected Test Result	Actual Test Result
Flame optics PMT Gain test		
For copper at 324.8 nm, 4 mA, 0.5 nm slit width	< 55 %	49 %
Flame performance test with 5 ppm copper sample		
Air /acetylene, mixing paddle removed	Abs value > 0.5	0.5599
Air /acetylene, mixing paddle installed, 10 replicates	%RSD < 1.0	0.2 %
Deuterium furnace optics PMT Gain test		
For copper at 324.8 nm, 4 mA, 0.5 nm slit width	< 55 %	—
Deuterium furnace performance test with 25 ppb copper sample (324.8 nm)		
Precision %RSD	≤ 4.0%	—
Abs value	≥ 0.15	—
Zeeman furnace analytical performance: 25 ppb copper sample (327.4 nm)		
Precision %RSD	≤ 4.0%	—
Abs value	≥ 0.10	—
MSRP%	≥ 70 %	—

Revision: 10.00, Issued: November 2021

© Agilent Technologies, Inc. 2021



AA consumable and parts list table

Part Description	Part Number	Product/Model # where used	PM supplied or Consumable	Instrument-Type
Test Solution – Cu 5ppm solution	6610030100	50 55 140 240 280	PM supplied	Common
Test Solution - Blank solution	5190-7001	50 55 140 240 280	PM supplied	Common
Copper, 1000 ug/ml, 100ml	5190-8279	50 55 140 240 280	*	Common
Kit, Mk 7 O-rings, aqueous, complete set	9910093400	50 55 140 240 280	PM supplied	Flame
Organic Kit	9910093500	50 55 140 240 280	PM supplied	Flame
Wire Nebulizer Cleaning	9910024700	50 55 140 240 280	consumable	Flame
Tubing-Capillary Std Nebs	9910024800	50 55 140 240 280	consumable	Flame
Capillary Tube Hivac Neb (3) (organics only)	9910044000	50 55 140 240 280	consumable	Flame
Glass impact beads (5/pk)	9910025700	50 55 140 240 280	consumable	Flame
Teflon impact beads (5/pk): (organics only)	9910053300	50 55 140 240 280	consumable	Flame
Burner cleaning strip (100/pk)	9910053900	50 55 140 240 280	consumable	Flame
Window UV silica – round (right side)	2010082600	50 55 140 240 280	PM supplied	Common
Window UV silica – rectangular (left side)	2010082500	50 55 140 240 280	PM supplied	Common
Pad adhesive window (round)	4910012700	50 55 140 240 280	PM supplied	Common
Pad adhesive window (rectangular)	4910012800	50 55 140 240 280	PM supplied	Common
Electrode kit (1 pr) (D2)	6310003400	GTA120	PM supplied	Furnace
Shroud (D2)	6310003100	GTA120	PM supplied	Furnace
Zeeman electrode kit (1 pr)	6310003500	GTA120	PM supplied	Furnace
Zeeman shroud	6310003600	GTA120	PM supplied	Furnace
O-ring PSD rinse bottle	6910025900	PSD120	PM supplied	Furnace

* For engineers who only service AA instruments 5190-8279 can be used as a cheaper alternative for 6610030100.

Items classified as PM supplied in the above table are included in the standard PM

Those classified as consumable should be provided by the customer or charged to the customer if supplied by the Agilent service engineer.

Revision: 10.00, Issued: November 2021

© Agilent Technologies, Inc. 2021



Service Engineer Comments (optional)

If there are any specific points you wish to note as part of performing the installation or other items of interest for the customer, please write in this box.

Report ID: Diagnostic Start Time: 1/30/2025 9:14:28 AM Diagnostic End Time: 1/30/2025 9:46:08 AM
Customer: UAE Service Engineer: Kanyakorn S.
Address: Soi Udomsuk 41, Sukhumvit Rd, Bangkok Contact Details: 026376363#1

Configuration:

Serial Number: MY13160001 Turret Type: Automatic
Instrument Model: Varian AA140/240/280 Number Of Lamps: 4
Flame Instrument: True Mono Type: Automatic
Furnace Instrument: True Gasbox Type: Y Gas Box
Zeeman Present: False Auto Burner Adjuster: False
Internal Zeeman: False Mains Frequency: 50
Internal UltraAA: False Firmware Version: 2.11
Optics Type: Double Beam Photomultiplier Type: Normal(900nm)
D2 BG Correction Fitted: True PWB Version: 45
Boot Block Version: 1.00

EEPROM Data:

Instrument Run Hours: 62819.180 D2 Run Hours: 53396.500
Zero Wavelength Offset: 0.133 D2 Serial Number: not set!
Mono Correction: 0.770 D2 Install Date: 1/1/1970
Flame Hours: 32411.634 D2 Original Intensity: 1.000
D2 Last Intensity: 475.000

Service Completion

Service request number: 6007549143 Date service completed: 30 Jan 2025
Agilent signature: Kanyakorn S. Customer signature: David Y.
Total number of pages in this document: 13

Frequency:

Averaging Period: 30.0
Datapoint Count: 20
Upper Limit: 51.00 Highest Measured Frequency: 50.00
Average Frequency: 50.00
Lower Limit: 49.00 Lowest Measured Frequency: 50.00
Result: Passed


Power Supply:

Averaging Period: 30.0
Datapoint Count: 20

	Lower Limit (V)	Actual (V)	Upper Limit (V)	Result:
12.00 V Rail	10.80	12.12	13.20	Passed
-12.00 V Rail	-13.20	-11.90	-10.80	Passed
5.00 V Rail	4.50	5.04	5.50	Passed
310.00 V Rail	279.00	330.00	341.00	Passed

Beam Balance:

Lamp Type: Copper
Lamp Socket Used: 3
Peak Selected: 324.80
Lamp Alignment: Performed

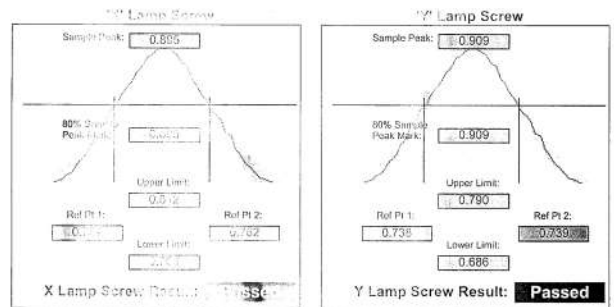

Grating Scan Results:

Lamp Element(s): Copper
Lamp Turret Position: 3
Lamp Current(mA): 4.00
Scan Wavelength(nm): 0.5
1st Order Wavelength(nm): 324.80
Lamp Alignment: Performed


	Lower Limit (nm)	Actual (nm)	Upper Limit (nm)	Result:
Zero Order	-0.10	0.00	0.10	Passed
First Order	324.45	324.75	325.15	Passed
Second Order	648.90	649.50	649.97	Passed

เอกสารไม่ควบคุม

Analyst:
Date Started: 1/30/2025 10:33 AM GMT: 1/30/2025 3:33 AM
Worksheet: Precision Test
Comment:
Methods: Cu
Computer name: DESKTOP-PSUFRS
Serial Number: MY13160001

Method: Cu (Flame)





Sample ID	Conc. mg/L	%RSD	Mean Abs
CAL ZERO	0.000	64.1	-0.0002
Readings	-0.0003	-0.0003	-0.0001
STANDARD 1	5.000	0.3	0.6052
Readings	0.6036	0.6073	0.6047

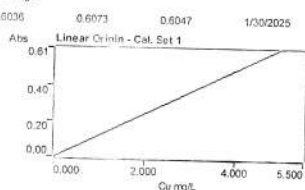

Curve Fit = Linear Origin
Characteristic Conc = 0.009 mg/L
r = 1.0000
Calculated Conc = -0.002 5.090
Residuals = 0.002 0.000

Abs = 0.12105 x C

5 ppm Cu	5.007	0.2	0.6051
Readings	0.6005	0.5952	0.6047
	0.6055	0.6076	0.6064
			0.6079
			1/30/2025 10:48:32 AM

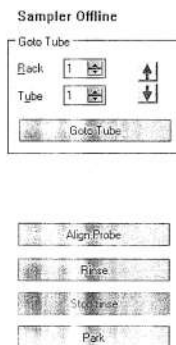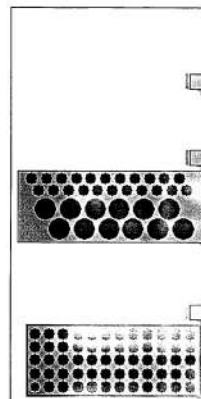

0.917

Optimize Lamp
Optimize Signal

Rescale

Inst Zero

Gain 49 %

Ok

Sensitivity Check 1.5 mg/L gives about 0.2 Abs at 324.8 nm, A/A burner

เอกสารไม่ควบคุม

เอกสารไม่ควบคุม



PinAAcle 900F Preventive Maintenance Report

Company Name: UAE Consultant Co., LTD.

Instrument Location: 41 Sukumvit Rd.,

Phra Khanong, Bangkok 10260

Instrument Serial No.: PFB520031902

Date: 29-Apr-2025

PinAAcle 900F Preventive Maintenance (PM)

Company Name:	United Analyst and Engineering Consultant Co., LTD.		
Address (Instrument Location):	41 Sukumvit Rd., Phra Khanong, Bangkok 10260		
Serial Number:	PFB520031902	PM Number:	1 of 2
Customer Name (if applicable):	K. Yinda	Telephone Number:	095-5580049
Customer Support Engineer Name:	K. Chayanon	Service Order Number:	WO-03126047
Date PM Performed: (DD-MM-YYYY)	29-Apr-2025	Next PM Due Date: (DD-MM-YYYY)	29-Oct-2025
Standard Labor Hours to Complete PM :		5 hours	

Part Number	Release	Publication Date	
09370145 Rev.9	A	January 2018	

Scope

The purpose of this PM is to ensure the continued functionality of the PinAAcle 900F by inspecting and replacing any worn or damaged parts. This service should only be performed by a trained representative of PerkinElmer.

The customer should save their method before the PM begins.

General Instructions:

The customer must provide the engineer operational data to demonstrate recent instrument performance prior to starting the PM.

Always check with the customer before making any changes that may affect the customer's analysis or calibration, including a current back-up of system software and/or data files.

The completed document should be signed by an authorized PerkinElmer and customer representative and left with the customer.

Update the PM sticker and instrument logbook as required.

Copyright Information

This document contains proprietary information that is protected by copyright. All rights are reserved. No part of this publication may be reproduced in any form whatsoever or translated into any language without the prior, written permission of PerkinElmer, Inc. Copyright © 2013 PerkinElmer, Inc.

Trademarks

Registered names, trademarks, etc. used in this document, even when not specifically marked as such, are protected by law. PerkinElmer is a registered trademark of PerkinElmer, Inc. All other trademarks and registered trademarks not owned by PerkinElmer, Inc. or its subsidiaries that are depicted herein are the property of their respective owners. Except as specifically set forth in its terms and conditions of sale, PerkinElmer makes no Warranty of any kind with regard to this document, including, but not limited to, the implied warranties of merchantability and fitness for a particular purpose. PerkinElmer shall not be liable for incidental or consequential damages in connection with the furnishing or use of this document.

เอกสารไม่ควบคุม

เอกสารไม่ควบคุม

Component List

Component / Specific Model	Serial #	Configuration Notes
PinAAcle900F	PFBS20031902	Syngistix V4.0.1.1935
FIAS100	100524040501	

Parts Lists

Parts Included with the PM		
Part Number (if applicable)	Description	Quantity
B0501696	Fan Filters	2
N3160156	O-Ring Kits for Sampling Introduction (Stainless Steels Nebulizer)	N/A
N3160157	O-Ring Kits for Sampling Introduction (Plastic Nebulizer)	1
N9301714	Replacement Acetylene Filter Cartridge	1
TH001022	Replacement Air Filter Cartridge	1

Additional Reagents and Standards Required for PM				
Part Number (if applicable)	Description	Quality	Batch/Lot #	Expired Date (MM/YY)
N9300183	1000 mg/L Copper Standard	AR	27-39CUY1	Nov 2025

Additional Reagents and Standards Required for PM (Customer Support Solution)				
Part Number (if applicable)	Description	Quantity	Batch/Lot #	Expiration Date (MM/YY)
N/A	DI Water	250 mL	AR	AR
N/A	0.5% HNO ₃	250 mL	AR	AR

เอกสารไม่ควบคุม

Procedure Checklist

Use (✓) to check off those steps in the checklist that have been completed.

1. General:

- ☒ Review the instrument performance with the customer and document any recent problems.
- ☒ Inspect the customer log book and make any appropriate PM entries.
- ☒ Perform general inspection of system for cleanliness.

2. PC Instrument Software:

- ☒ Instrument Software user files/databases archived, packed, and/or deleted as needed.

3. Mechanical:

- ☒ Inspect and clean all fans and filters. Replace filters if necessary
- ☒ Inspect all gas lines for leaks and/or wear. Replace if needed.
- ☒ Clean exterior of the instrument.
- ☒ Inspect the burner head, burner chamber, and nebulizer. Clean if needed as stated in the Hardware Guide.
- ☒ Check burner head dimensions with the feeler gauge as stated in the Hardware Guide in the Maintenance chapter section on cleaning the burner head and checking sloth width. Replace if out of specification
- ☒ Check the condition of the end cap, burner head, and nebulizer O-rings. Replace if necessary.
- ☒ Check the drain system for signs of wear. Replace worn or damaged parts.
- ☒ Visually check for proper flame conditions when igniting the Air-C2H2 and N2O-C2H2 flames (if applicable).

4. Electrical:

- ☒ Inspect PC boards. Clean if necessary.
- ☒ Carefully check all internal and external cable connections.
- ☒ Check instrument firmware revisions upgrade to current levels (if necessary)
- ☒ Run Diagnostics Test within the Advanced function of the Spectrometer page. Check the results in the service log folder in the Spectrometer BM Log Viewer.

5. Optics:

- ☒ Inspect and clean the sample compartment windows, if needed.
- ☒ Inspect optics. Clean or replace if necessary.

6. Gasses:

- ☒ Verify that the Gasses supplied to the instrument are within the pressure and purity specifications found in the PinAAcle 900 Series Pre-Installation Checklist SDB.
- ☒ Verify that the acetylene filter and air filter element is dry. Replace if necessary.

เอกสารไม่ควบคุม

Additional Tools Required for PM

Part Number (if applicable)	Description	Quantity	Serial #
N1013000	0.2A Neutral density filter	1	101N0089015
N1013002	1.0A Neutral density filter	1	101N0089015
03030997	System 2 EDL Driver	1	03030997
N3050605	As System 2 EDL	1	16148
N3050121	Cu Lumina HCL	1	060419-030180
N3050109	Ba Lumina HCL	1	061219-020041
N3050139	K Lumina HCL	1	030819-010130
N3050152	Ni Lumina HCL	1	052719-020020

เอกสารไม่ควบคุม

7. Flame Interlock Check:

Description: Check to ensure that all safety interlocks are closed.

Parameter	Specification	Test Results	Pass/Fail
Flame Sensor	Air/C ₂ H ₂ Flame correctly shuts down	Active	Passed
Drain Sensor	Air/C ₂ H ₂ Flame correctly shuts down	Active	Passed
Nebulizer Sensor	Air/C ₂ H ₂ Flame correctly shuts down	Active	Passed
C ₂ H ₂ Pressure Sensor	Air/C ₂ H ₂ Flame correctly shuts down	Active	Passed
Air Pressure Sensor	Air/C ₂ H ₂ Flame correctly shuts down	Active	Passed
Burner Head Sensor	Choosing Nitrous Oxide as the oxidant should trigger an interlock shuts down	Active	Passed

8. After PM Performance tests:

8.1 Detector Linearity with Barium

Description: Ensures that the detector is linear in the Visible Range.

Parameter	Specification	Certificate Value at 553.6 nm (Abs.)	Test Results	Pass/Fail
1.0 A ND Filter	± 5% from Cert.	0.9668	0.9878	Passed
0.2 A ND Filter	± 5% from Cert.	0.1953	0.1876	Passed

8.2 Baseline Noise at 1.0 Absorbance with Barium

Description: Ensures that a high absorbance will not produce excessive noise.

Parameter	Specification	Results	Pass/Fail
Standard Deviation	≤ 0.010	0.0005	Passed

8.3 AA Baseline Noise with Copper

Description: Check baseline noise.

Parameter	Specification	Results	Pass/Fail
Standard Deviation	≤ 0.001	0.0001	Passed

เอกสารไม่ควบคุม

8.4 D₂ Background Compensation with Copper

Description: Verifies the instruments ability to compensate for Background absorption.

Parameter	Specification	Results	Pass/Fail
Standard Deviation	≤ 0.010	0.009	Passed

8.5 AA-BG Baseline Noise with Copper

Description: Ensures that background correction does not produce excessive noise.

Parameter	Specification	Results	Pass/Fail
Standard Deviation	≤ 0.005	0.0001	Passed

8.6 AA-BG Baseline Noise with Arsenic

Description: Ensures that background correction does not produce excessive noise at a low wavelength.

Parameter	Specification	Results	Pass/Fail
Standard Deviation	≤ 0.005	0.0004	Passed

8.7 Flame Sensitivity

Description: Instrument Sensitivity checked against Copper standard.

Standard Copper Sensitivity	Specification	Results (Abs.)	Pass/Fail
5 mg/L Sensitivity SS Neb (if applicable)	> 0.250 Abs.	N/A	Not Applicable
2 mg/L Sensitivity HS Neb (if applicable)	> 0.250 Abs.	N/A	Passed

10. Review:

- ☒ Review with the customer PM work performed.
☒ Review with the customer routine maintenance procedures.
☒ Discuss recommended customer supplied materials to have on hand.
☒ Attach PM sticker.

Additional Comments

Additional Comments Regarding the PM

Review

The preventive maintenance checks and if applicable performance tests for PinAAcle 900F have been completed.

This PinAAcle 900F Passes ☒ Fails ☐ the preventive maintenance.

Review of Preventive Maintenance:

Authorized PerkinElmer Representative: <i>Chayanon K.</i>	Date: 29 Apr 2025 (DD-MMM-YYYY)
Authorized Customer Representative: <i>Syinhom</i>	Date: 29 Apr 2025 (DD-MMM-YYYY)

PinAAcle 900F Preventive Maintenance Report (PM)

Page 6 of 7

PinAAcle 900F Preventive Maintenance Report (PM)

Page 7 of 7

เอกสารไม่ควบคุม

เอกสารไม่ควบคุม



PerkinElmer Scientific (Thailand) Co., Ltd.
290 Soi Soomvijai 4
Khwaeng Bangkok, Khet Huay Kwang
Bangkok 10310
Thailand
Tel: 66 2719 6420 ; Fax: +66 2 319 7900
http://www.perkinelmer.com

Service Report

Service Report					
Work Order Number	Activity Code	Billing Type	Requested Start Date	Model	Serial Number
WO-03126047	Planned Maintenance	Contract	10/01/2568 11:08 u.	AAN3200551	PFB520031902
Service Representative Name		Contract Number	Expiry Date	Equipment ID	System ID
Kanan, Chayanon		SC-0035964109	31/10/2025	N/A	N/A
UDI Number					
N/A					
Equipment Location			SI To Name		
บริษัท ชัยนาท เทคโนโลยี จำกัด อาคาร 51 ถนนพหลโยธิน กรุงเทพมหานคร 10260 TH			บริษัท ชัยนาท เทคโนโลยี จำกัด อาคาร 51 ถนนพหลโยธิน กรุงเทพมหานคร 10260 TH		
Customer Contact	Phone Number	Fax Number	Email	Purchase Order	
K. ญาณาน ชัยนาท (นาย)	795-5580049	N/A	nichakom.prasert1999@gmail.com	HPO-230100002	

Work Description

PM 2/2 (Main/Service) - Cleaning Cell, Chamber, Filter - Wavelength Calibrate : Pass - Wavelength Scan As.Cu.Ba.K.Ni : Pass - Align cell with Hg : OK	Work Description
Start Date 28/04/2025	End Date 08/05/2025

Tools Used

Quantity	Calibrated Tool	Description	Serial Number	Last Calibration Date	Next Calibration Date
*** No Calibrated Tools Used ***					

Material Used

Part Number	Part Description	Note	Lot/Serial Number	Quantity
*** No Parts Used ***				

Labour Details

Part Number	Description	Start Date	Quantity
SVB00013	Preventative maintenance	28/04/2025	4

Work Complete Yes <input checked="" type="checkbox"/> No <input type="checkbox"/>	Customer Signature <i>ญาณาน</i> 9/52568 K. ญาณาน ชัยนาท (นาย)	Technician Signature <i>Chayanon K.</i> 9/52568 Kanan, Chayanon
PMOQ/PIV Left with Customer Yes <input type="checkbox"/> No <input checked="" type="checkbox"/>		

Terms & Conditions

เอกสารไม่ควบคุม

Customer Acknowledgment of receipt of the above repair / replacement.

Special Terms and Conditions: This is not an invoice.


Terms will be applied to your invoice if applicable.

9/52568 WO-03126047

Page 2 of 2

เอกสารไม่ควบคุม

Atomic Absorption/FIAS 100/400 Preventive Maintenance (PM)			
Company Name:	United Analyst and Engineering Consultant Co., LTD.		
Address (Instrument Location):	41 Sukumvit Rd., Phra Khanong, Bangkok 10260		
Room Number:	Lab		
Asset Number (if applicable):	2 of 2W	Customer System ID:	K. Yanida
Service Engineer Name:	K. Chayanan	Service Order Number:	WO-03051971
Date PM Performed: (DD-MMM-YYYY)	29-Apr-2025	Next PM Due Date: (DD-MMM-YYYY)	29-Oct-2025

Part Number	Release	Publication Date	
09370005	C	January 2013	

Scope

The purpose of this PM is to ensure the continued functionality of the Atomic Absorption/FIAS 100/400 by inspecting and replacing any worn or damaged parts. This service should only be performed by a trained representative of PerkinElmer. The customer should save their method before the PM begins.

General Instructions:

Always check with the customer before making any changes that may affect the customer's analysis or calibration. The completed document should be signed by an authorized PerkinElmer and customer representative and left with the customer. Update the PM sticker and instrument logbook as required.

Copyright Information

This document contains proprietary information that is protected by copyright. All rights are reserved. No part of this publication may be reproduced in any form whatsoever or translated into any language without the prior, written permission of PerkinElmer, Inc. Copyright © 2013 PerkinElmer, Inc.

Trademarks

Registered names, trademarks, etc. used in this document, even when not specifically marked as such, are protected by law. PerkinElmer is a registered trademark of PerkinElmer, Inc. All other trademarks and registered trademarks not owned by PerkinElmer, Inc. or its subsidiaries that are depicted herein are the property of their respective owners. Except as specifically set forth in its terms and conditions of sale, PerkinElmer makes no warranty of any kind with regard to this document, including, but not limited to, the implied warranties of merchantability and fitness for a particular purpose. PerkinElmer shall not be liable for incidental or consequential damages in connection with the furnishing or use of this document.

Component List

Component / Specific Model	Serial #	Firmware Version	Configuration Notes
FIAS100	100S24040501	2.20	Syngistix V4.0.1.1935

Parts Lists

Parts Included with the PM				
Part Number (if applicable)	Description	Quantity	Batch/Lot #	Expiration Date (MM/YY)
B050 2706	Fan Filter	1	N/A	N/A

Additional Tools Required for PM				
Part Number (if applicable)	Description	Quantity	Serial #	Calibration Due Date (MM/YY)
N/A	Digital Volt Meter	1	N/A	N/A

Additional Reagents and Standards Required for PM				
Part Number (if applicable)	Description	Quantity	Batch/Lot #	Expiration Date (MM/YY)
N/A	N/A	N/A	N/A	N/A

เอกสารไม่ควบคุม

เอกสารไม่ควบคุม

Procedure Checklist

Use (✓) to check off those steps in the checklist that have been completed.

1. General:

- ☒ Review the instrument performance with the customer and document any recent problems.

- ☒ Is the Working Environment Acceptable? If not, document.

- ☐ Visual Damage (if yes, describe)

- ☒ Check incoming AC line voltage for proper levels and grounding.
☒ Verify Voltage switch on back of instrument is correct.
☒ Perform general inspection of system for cleanliness. Clean if needed.
☒ Gas supply cylinders secured, lines leak checked and argon or nitrogen supply pressure verified (45 – 58 psi).
☒ Inspect the customer log book and make any appropriate PM entries.
☒ Fan checked and filter cleaned
☒ Heating mantle or Universal Cell Holder checked

2. Instrument components

- ☒ Non-return valve checked/repared/replaced if needed (B019 8111). Clean the valve if there is any liquid in it. Replace the rubber sleeve (B013 5123) if it is worn. Check the flow meter for any signs of fluid in it. Clean the flow meter if needed.
☒ Verify condition of pump pressure adjustment levers (B050 7794 - look for cracks or problems with the springs), pump rollers (B300 0251 check for wear), and thumb screws (B050 7796).
☒ Check the Multiport valve for proper switching, flow, and insure there are no leaks. Clean valve parts and replace o-rings if needed (large o-ring: B050 1250, small o-ring: B004 5095). Use a squirt bottle & fishing line to try to dislodge clogs.
☒ Firmware Version checked. Latest is 2.20.

3. Mixing/Separation Assembly & Pump Tubing:

- ☒ Mixing separator assembly checked
☒ Filter/membrane checked (B050 8306)
☒ Condition of the pump tubing (replace if necessary), correct pump tubing for the solutions being run. Make sure the correct magazines are being used. B050 7791 for 0.13 – 1.80 mm tubing; B050 7792 for 1.60 – 3.18 mm tubing.

4. Cell, Cell Windows, Transfer Line:

- ☒ Cell checked
☒ Cell windows checked
☒ Transfer line checked for moisture (if moisture is a problem, the Nafion dryer might be needed)

5. Operational Tests:

- ☒ Run DI water through the carrier/reductant/sample system. Verify smooth flow of liquid throughout without leaks. Replace tubing & fittings if needed.

6. Review:

- ☒ Review with the customer PM work performed.
☒ Review with the customer routine maintenance procedures.
☒ Discuss recommended customer-supplied materials to have on hand.
☒ Attach PM sticker.
☒ Update Logbook.

เอกสารไม่ควบคุม

เอกสารไม่ควบคุม

Additional Comments

Additional Comments Regarding the PM

Document History

Revision	Description of Change	Page(s)	Date
A	First release		May 2008
B	Addition of Batch/Lot Number, Expiration Date, and Report Fields.	2,7	February 2009
C	Update to new format	All	January 2013

Review

The preventive maintenance checks and if applicable performance tests for FIAS 100/400 have been completed.	
This FIAS 100/400 Passes <input checked="" type="checkbox"/> Fails <input type="checkbox"/> the preventive maintenance.	
Review of Preventive Maintenance:	
Authorized PerkinElmer Representative: <i>Chayman k.</i>	Date: 29 Apr 2025 (DD-MMM-YYYY)
Authorized Customer Representative: <i>สุวิทย์ หงษา</i>	Date: 29 Apr 2025 (DD-MMM-YYYY)

เอกสารไม่ควบคุม

เอกสารไม่ควบคุม



PerkinElmer Scientific (Thailand) Co., Ltd.
290 Soi Sornvijai 4
Khwang Bangkapi, Khat Huay Kwang
Bangkok 10310
Thailand
Tel: 66 2719 6420 ; Fax: +66 2 319 7900
http://www.perkinelmer.com

Customer Acknowledgment of receipt of the above repair / replacement.
Special Terms and Conditions: This is not an invoice.
Taxes will be applied to your invoice if applicable.

Service Report

Work Order Number	Activity Code	Billing Type	Requested Start Date	Model	Serial Number
WG-03051971	Planned Maintenance	Contract	10/03/2568 23.06 u.	B0508570	100524040501
Service Representative Name	Contract Number	Expiry Date	Equipment ID	System ID	
Kanan, Chayanon	SC-003569090	24/05/2025	N/A	N/A	
UDI Number					
N/A					
Equipment Location			BI To Name		
บริษัท สุวิทย์ หงษา จำกัด อาคารพาณิชย์ 51/10260 TH			บริษัท สุวิทย์ หงษา จำกัด อาคารพาณิชย์ 51/10260 TH		
Customer Contact	Phone Number	Fax Number	Email	Purchase Order	
K. Nitchakorn วนะวิตรู	085-5580568	N/A	perkitohar42@gmail.com	HPO-240400211	

Work Description	
- PM 212 Warranty - Cleaning Port Vals, Manifold, Tuning - Run Hg test : Pass Start Date: 29/04/2025 End Date: 29/04/2025 Work Description:	

Tools Used				
Quantity	Calibrated Tool	Description	Serial Number	Last Calibration Date
*** No Calibrated Tools Used ***				

Material Used				
Part Number	Part Description	Note	Lot/Serial Number	Quantity
*** No Parts Used ***				

Labour Details			
Part Number	Part Description	Start Date	Quantity
SV000013	Preventative maintenance	29/04/2025	3
SV000002	Service Travel	29/04/2025	1

Work Complete	Customer Signature	Technician Signature
Yes <input checked="" type="checkbox"/> No <input type="checkbox"/> PM/QIPV Left with Customer Yes <input type="checkbox"/> No <input checked="" type="checkbox"/>	<i>สุวิทย์ หงษา</i>	<i>Chayman k.</i>
	95/2568 K. Nitchakorn วนะวิตรู	95/2568 Kanan, Chayanon

Terms & Conditions

เอกสารไม่ควบคุม

เอกสารไม่ควบคุม

Terms & Conditions

Customer Acknowledgment of receipt of the above repair / replacement.
Special Terms and Conditions: This is not an invoice.
Taxes will be applied to your invoice if applicable.



PinAAcle 900F
Preventive Maintenance Report

Company Name:UAE Consultant Co., LTD.
Instrument Location: 41 Sukumvit Rd.,
Phra Khanong, Bangkok 10260
Instrument Serial No.:PFBS20031902
Date: 14-May-2024

9/5/2568 WO-03126049

Page 2 of 2

เอกสารไม่ควบคุม

เอกสารไม่ควบคุม

PinAAcle 900F Preventive Maintenance (PM)

Company Name:	United Analyst and Engineering Consultant Co., LTD.		
Address (Instrument Location):	41 Sukumvit Rd., Phra Khanong, Bangkok 10260		
Serial Number:	PFBS20031902	PM Number:	2 of 2
Customer Name (if applicable):	K. Yalinda	Telephone Number:	095-5580049
Customer Support Engineer Name:	K. Chayanan	Service Order Number:	WO-02787590
Date PM Performed: (DD-MM-YYYY)	14-May-2024	Next PM Due Date: (DD-MM-YYYY)	14-Nov-2024
Standard Labor Hours to Complete PM :		5 hours	

Part Number	Release	Publication Date	
09370145 Rev.9	A	January 2018	

Scope

The purpose of this PM is to ensure the continued functionality of the PinAAcle 900F by inspecting and replacing any worn or damaged parts. This service should only be performed by a trained representative of PerkinElmer.

The customer should save their method before the PM begins.

General Instructions:

The customer must provide the engineer operational data to demonstrate recent instrument performance prior to starting the PM.

Always check with the customer before making any changes that may affect the customer's analysis or calibration, including a current back-up of system software and/or data files.

The completed document should be signed by an authorized PerkinElmer and customer representative and left with the customer.

Update the PM sticker and instrument logbook as required.

Copyright Information

This document contains proprietary information that is protected by copyright. All rights are reserved.

No part of this publication may be reproduced in any form whatsoever or translated into any language without the prior, written permission of PerkinElmer, Inc.

Copyright © 2013 PerkinElmer, Inc.

Trademarks

Registered names, trademarks, etc. used in this document, even when not specifically marked as such, are protected by law. PerkinElmer is a registered trademark of PerkinElmer, Inc. All other trademarks and registered trademarks not owned by PerkinElmer, Inc. or its subsidiaries that are depicted herein are the property of their respective owners. Except as specifically set forth in its terms and conditions of sale, PerkinElmer makes no Warranty of any kind with regard to this document, including, but not limited to, the implied warranties of merchantability and fitness for a particular purpose.

PerkinElmer shall not be liable for incidental or consequential damages in connection with the furnishing or use of this document.

Component List

Component / Specific Model	Serial #	Configuration Notes
PinAAcle900F	PFBS20031902	Syngistix V.4.0.1.1935
Fias100(New Install)	100524040501	

Parts Lists

Parts Included with the PM		
Part Number (if applicable)	Description	Quantity
B0501696	Fan Filters	N/A
N3160156	O-Ring Kits for Sampling Introduction (Stainless Steels Nebulizer)	N/A
N3160157	O-Ring Kits for Sampling Introduction (Plastic Nebulizer)	N/A
N9301714	Replacement Acetylene Filter Cartridge	N/A
TH001022	Replacement Air Filter Cartridge	N/A

Additional Reagents and Standards Required for PM

Part Number (if applicable)	Description	Quality	Batch/Lot #	Expired Date (MM/YY)
N9300183	1000 mg/L Copper Standard	AR	27-39CUY1	Apr 2025

Additional Reagents and Standards Required for PM (Customer Support Solution)

Part Number (if applicable)	Description	Quantity	Batch/Lot #	Expiration Date (MM/YY)
N/A	DI Water	250 mL	AR	AR
N/A	0.5% HNO ₃	250 mL	AR	AR

เอกสารไม่ควบคุม

เอกสารไม่ควบคุม

Procedure Checklist

Use (✓) to check off those steps in the checklist that have been completed.

1. General:

- ☒ Review the instrument performance with the customer and document any recent problems.
- ☒ Inspect the customer log book and make any appropriate PM entries.
- ☒ Perform general inspection of system for cleanliness.

2. PC Instrument Software:

- ☒ Instrument Software user files/databases archived, packed, and/or deleted as needed.

3. Mechanical:

- ☒ Inspect and clean all fans and filters. Replace filters if necessary.
- ☒ Inspect all gas lines for leaks and/or wear. Replace if needed.
- ☒ Clean exterior of the instrument.
- ☒ Inspect the burner head, burner chamber, and nebulizer. Clean if needed as stated in the Hardware Guide.
- ☒ Check burner head dimensions with the feeler gauge as stated in the Hardware Guide in the Maintenance chapter section on cleaning the burner head and checking sloth width. Replace if out of specification.
- ☒ Check the condition of the end cap, burner head, and nebulizer O-rings. Replace if necessary.
- ☒ Check the drain system for signs of wear. Replace worn or damaged parts.
- ☒ Visually check for proper flame conditions when igniting the Air-C2H2 and N2O-C2H2 flames (if applicable).

4. Electrical:

- ☒ Inspect PC boards. Clean if necessary.
- ☒ Carefully check all internal and external cable connections.
- ☒ Check instrument firmware revisions upgrade to current levels (if necessary)
- ☒ Run Diagnostics Test within the Advanced function of the Spectrometer page. Check the results in the service log folder in the Spectrometer BM Log Viewer.

5. Optics:

- ☒ Inspect and clean the sample compartment windows, if needed.
- ☒ Inspect optics. Clean or replace if necessary.

6. Gasses:

- ☒ Verify that the Gasses supplied to the instrument are within the pressure and purity specifications found in the PinAAcle 900 Series Pre-installation Checklist SDB.
- ☒ Verify that the acetylene filter and air filter element is dry. Replace if necessary.

เอกสารไม่ควบคุม

เอกสารไม่ควบคุม

7. Flame Interlock Check:

Description: Check to ensure that all safety interlocks are closed.

Parameter	Specification	Test Results	Pass/Fail
Flame Sensor	Air/C ₂ H ₂ Flame correctly shuts down	Active	Passed
Drain Sensor	Air/C ₂ H ₂ Flame correctly shuts down	Active	Passed
Nebulizer Sensor	Air/C ₂ H ₂ Flame correctly shuts down	Active	Passed
C ₂ H ₂ Pressure Sensor	Air/C ₂ H ₂ Flame correctly shuts down	Active	Passed
Air Pressure Sensor	Air/C ₂ H ₂ Flame correctly shuts down	Active	Passed
Burner Head Sensor	Choosing Nitrous Oxide as the oxidant should trigger an interlock shuts down	Active	Passed

8. After PM Performance tests:

8.1 Detector Linearity with Barium

Description: Ensures that the detector is linear in the Visible Range.

Parameter	Specification	Certificate Value at 553.6 nm (Abs.)	Test Results	Pass/Fail
1.0 A ND Filter	± 5% from Cert.	0.9995	1.0143	Passed
0.2 A ND Filter	± 5% from Cert.	0.1936	0.1966	Passed

8.2 Baseline Noise at 1.0 Absorbance with Barium

Description: Ensures that a high absorbance will not produce excessive noise.

Parameter	Specification	Results	Pass/Fail
Standard Deviation	≤ 0.010	0.002	Passed

8.3 AA Baseline Noise with Copper

Description: Check baseline noise.

Parameter	Specification	Results	Pass/Fail
Standard Deviation	≤ 0.001	0.0002	Passed

8.4 D₂ Background Compensation with Copper

Description: Verifies the instruments ability to compensate for Background absorption.

Parameter	Specification	Results	Pass/Fail
Standard Deviation	≤ 0.010	0.0001	Passed

8.5 AA-BG Baseline Noise with Copper

Description: Ensures that background correction does not produce excessive noise.

Parameter	Specification	Results	Pass/Fail
Standard Deviation	≤ 0.005	0.002	Passed

8.6 AA-BG Baseline Noise with Arsenic

Description: Ensures that background correction does not produce excessive noise at a low wavelength.

Parameter	Specification	Results	Pass/Fail
Standard Deviation	≤ 0.005	0.0022	Passed

8.7 Flame Sensitivity

Description: Instrument Sensitivity checked against Copper standard.

Standard Copper Sensitivity	Specification	Results (Abs.)	Pass/Fail
5 mg/L Sensitivity SS Neb (if applicable)	> 0.250 Abs.	N/A	Not Applicable
2 mg/L Sensitivity HS Neb (if applicable)	> 0.250 Abs.	0.8005	Passed

10. Review:

- ☒ Review with the customer PM work performed.
- ☒ Review with the customer routine maintenance procedures.
- ☒ Discuss recommended customer supplied materials to have on hand.
- ☒ Attach PM sticker.

เอกสารไม่ควบคุม

เอกสารไม่ควบคุม

Additional Comments

Additional Comments Regarding the PM

Review

The preventive maintenance checks and if applicable performance tests for PinAAcle 900F have been completed.

This PinAAcle 900F Passes ☒ Fails ☐ the preventive maintenance.

Review of Preventive Maintenance:

Authorized PerkinElmer Representative:	Date:
Chayaman K.	14-May-2024 (DD-MM-YYYY)
Authorized Customer Representative:	Date:
สุวิทย์ น้อย	14-May-2024 (DD-MM-YYYY)

PinAAcle 900F Preventive Maintenance Report (PM)

Page 7 of 7

เอกสารไม่ควบคุม



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL.0-2717-3000-29 FAX.0-2719-9484



Certificate of Calibration

Cert.No.: 24MM292
Page.: 1 of 3

Equipment : Electronic Balance
Manufacturer : Mettler Toledo
Model : AB204-S/FACT
Serial No. : 1129361010
ID No. : UAE.WAS.002/2552
Submitted by : United Analyst and Engineering Consultant Co.,Ltd.
3 Sol Udomsuk 41, Sukhumvit Road,
Bangchak, Phrakhanong,
Bangkok 10260
Location : Balance Room (108)
Received order : 11 May 2024
Calibration Date : 11 May 2024
Ambient Temperature : 15 °C to 40 °C
Relative Humidity : 30 % to 90 %
Calibrated by : Khit Ruttanaprapachai
Approved by : Kunchit
Approved Signatory
() Ponpan Paipim
() Suwit Imjai
(✓) Kunchit Promprat

Issue Date : 15 May 2024

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written Approval of the head of Corporate Services 3: Equipment Calibration and Testing Services.

เอกสารไม่ควบคุม



Equipment : Electronic Balance
Condition As-Received : Used Item
Reference : 2405-0166OC-1

Cert.No.: 24MM292
Page: 2 of 3

Procedure used :-

Calibration were conducted using in-house calibration procedure CP-OB01 based on UKAS LAB 14 according to direct measurement method against standard weight.

Condition of this result of calibration

1. Reference standard instruments:-

Instruments	Model	Serial No.	ID No.	Test report No.	Due date
1) Standard Weight Set (E2)	15884	24053	70RC007	MM-0013-24	25 Jan 2026

- This certificate is valid only to the item calibrated on date and place of calibration.
- This result of calibration was made on requested at the point specified by customer.
- This certificate is not certified for any commercial transaction.
- This certificate is traceable to the International System of Unit.

Result of calibration () Without Adjustment (*) After Adjustment by Internal Calibration

Range capacity : 0 g to 220 g Resolution 0.0001 g

Before Adjustment :

Applied Weight	Balance Reading	Correction	Measurement Uncertainty	Coverage Factor
(g)	(g)	(g)	(± mg)	(k)
100	100.0000	0.0000	0.19	2.03
200	200.0006	-0.0006	0.30	2

After Adjustment :

1. Determination of the standard deviation of weighing machine (n = 10)

Applied Weight	Standard Deviation of Reading (g)
(g)	
100	0.00007
200	0.00005



Equipment : Electronic Balance
Condition As-Received : Used Item
Reference : 2405-0166OC-1


Cert.No.: 24MM292
Page: 3 of 3

Result of calibration

2. Effect of off center loading

A mass of 100 g was placed to various position on the pan.
The weighing machine reading error obtained is given in the table

Position 1	Position 2	Position 3	Position 4	Position 5
(g)	(g)	(g)	(g)	(g)
-0.0004	-0.0004	-0.0003	-0.0003	-0.0004



Maximum difference between off-center and central loading (g)
0.0001

3. Departure from nominal value

Applied Weight	Balance Reading	Correction	Measurement Uncertainty	Coverage Factor
(g)	(g)	(g)	(± mg)	(k)
Unload	0.0000	0.0000	0.15	2.13
0.01	0.0100	0.0000	0.15	2.13
0.05	0.0500	0.0000	0.15	2.13
0.1	0.1000	0.0000	0.15	2.13
0.5	0.5000	0.0000	0.15	2.13
1	1.0000	0.0000	0.15	2.13
10	10.0000	0.0000	0.15	2.11
50	49.9999	+0.0001	0.17	2.06
100	99.9999	+0.0001	0.19	2.03
150	149.9998	+0.0002	0.29	2
200	199.9990	+0.0010	0.30	2

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k , providing a level of confidence of approximately 95 %.

-o0o-

เอกสารไม่ควบคุม

เอกสารไม่ควบคุม

Calibration Certificate

Certificate No.: 2402283-002-01
Client name: UNITED ANALYST AND ENGINEERING CONSULTANT CO., LTD.
Address: 3 SOI UDOMSUK 41, SUKHUMVIT ROAD,
Bangchack, Prakhong, Bangkok 10260

Page 1 of 4

Equipment: Electronic Balance
Manufacturer: METTLER TOLEDO
Model: XSR205DU
Serial No.: C210685394
ID No.: UAE.WAO.010/2565
Order No.: 2402283
Operation No.: 2402283-002
Date of Receipt: 2 April 2024
Date of Calibration: 2 April 2024

Calibrated by Mr.Jerawut Prapawuttipong
Scientist
Approved by (Mr.Pheraphat Tuanjit)
Manager, Division of Calibration Laboratory
Responsible for the Technical Management Team
Date of Issue: 9 April 2024

The uncertainties are for a confidence probability of approximately 95%

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full, except with the prior written approval of the National Food Institute.

F-CS-009 Revision: 01 Date: 20-04-65

เอกสารไม่ควบคุม



Calibration Report

Certificate No.: 2402283-002-01
Equipment: Electronic Balance
Model: XSR205DU
Serial No.: C210685394
Capacity: 220 g
Manufacturer: METTLER TOLEDO
Resolution: 0.00001 g / 0.0001 g
ID No.: UAE.WAO.010/2565

Page 2 of 4

Date of Calibration: 2 April 2024
Environment Condition: Ambient Temperature: 24.5 ± 0.5 °C Relative Humidity: 47.5 ± 2.5 %
Place of Calibration: Laboratory, UNITED ANALYST AND ENGINEERING CONSULTANT CO., LTD.
Condition of Equipment: Good Condition

Condition of This Results of Calibration:
1. Calibration Method: NFI Method W-MA-001 In-House Method based on UKAS Lab 14 : 2019

Reference Standard	Model	Serial No.	Calibrated By	Certificate No.	Due Date
Standard Weight Class E2	1mg to 200g	8505567572	TCS	M23040535	8 April 2024
Instrument	Model	Serial No.	Calibrated By	Certificate No.	Due Date
Thermo-Hygro Meter	608-H3	NFLBTH 016/23	Quality Reborn	QB24-0343	9 February 2025

3. This certification is traceable to SI UNIT
4. This certificate was certified only for the instrument we calibrated.
5. This result of calibration was found accurate as shown on date and place of calibration only.


Calibration Results:

1. Repeatability of Reading:

Nominal Value (g)	Standard Deviation of Reading (g)
40	0.0000042
80	0.0000052
100	0.000048
200	0.000548

2. Off-Center Error:

A mass of 100 g was placed and moved to various position on pan.
The balance reading obtained is given in the table.



1	2	3	4	5	6	(Maximum Difference)
(g)	(g)	(g)	(g)	(g)	(g)	(g)
100.0000	100.0001	99.9999	99.9999	100.0001	100.0000	0.0001

F-CS-012 Revision: 01 Date: 20-04-65

เอกสารไม่ควบคุม



Calibration Report

Certificate No.: 2402283-002-01
Equipment: Electronic Balance
Model: XSR205DU
Serial No.: C210685394
Capacity: 220 g
Manufacturer: METTLER TOLEDO
Resolution: 0.00001 g / 0.0001 g
ID No.: UAE.WAO.010/2565

Date of Calibration: 2 April 2024
Page 3 of 4

Calibration Results: (Continued)

Calibration Range: 0 - 80 g

Calibration Adjustment: Internal Calibration

3. Departure from Nominal Value: (Range: 0 - 80 g ; Resolution: 0.00001 g)

Nominal Value (g)	Standard Value (g)	Average Reading (g)	Correction (g)	Uncertainty (± g)	Coverage Factor
Unload	0.000000	0.000000	0.000000	0.0000086	2.00
0.001	0.001003	0.00101	-0.00001	0.0000089	2.00
0.005	0.005003	0.005000	0.000003	0.0000092	2.00
0.01	0.010003	0.010000	0.000003	0.0000089	2.00
0.05	0.049996	0.050000	0.000004	0.0000096	2.00
0.1	0.100011	0.100000	0.000011	0.000011	2.00
0.5	0.500016	0.500001	0.000015	0.000014	2.00
1	1.000003	1.000002	-0.000001	0.000016	2.00
2	2.000023	2.000001	0.000022	0.000017	2.00
5	5.000017	5.000002	0.000015	0.000020	2.00
10	10.000009	10.000000	0.000009	0.000026	2.00
20	20.000031	20.000000	0.000031	0.000037	2.00
30	30.000040	30.000001	0.000039	0.000050	2.00
50	50.000028	50.000002	0.000026	0.000068	2.00
80	80.000068	80.000002	0.000066	0.00011	2.00

F-CS-012 Revision: 01 Date: 20-04-65

เอกสารไม่ควบคุม



Calibration Report

Certificate No.: 2402283-002-01
Equipment: Electronic Balance
Model: XSR205DU
Serial No.: C210685394
Capacity: 220 g
Manufacturer: METTLER TOLEDO
Resolution: 0.00001 g / 0.0001 g
ID No.: UAE.WAO.010/2565

Page 4 of 4

Calibration Results: (Continued)

Calibration Range: 81 - 200 g

Calibration Adjustment: Internal Calibration

3. Departure from Nominal Value: (Range: 81 - 200 g ; Resolution: 0.0001 g)

Nominal Value (g)	Standard Value (g)	Average Reading (g)	Correction (g)	Uncertainty (± g)	Coverage Factor
90	90.000010	90.00001	0.000000	0.00015	2.00
100	100.000006	100.00001	0.000004	0.00015	2.00
110	110.000007	110.00001	0.000003	0.00016	2.00
120	120.000009	120.00000	0.000009	0.00017	2.00
130	130.000010	130.00000	0.000010	0.00019	2.00
140	140.000014	140.00000	0.000014	0.00020	2.00
150	150.000009	150.00001	0.000001	0.00020	2.00
160	160.000019	160.00001	0.000000	0.00022	2.00
170	170.000012	170.00001	0.000000	0.00023	2.00
200	200.000016	200.00002	0.000004	0.00028	2.00

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k, providing a level of confidence of approximately 95 %.

F-CS-012 Revision: 01 Date: 20-04-65

เอกสารไม่ควบคุม



Calibration Certificate

Certificate No.: 2402283-001-01
Client name: UNITED ANALYST AND ENGINEERING CONSULTANT CO., LTD.
Address: 3 Soi Udumuk 41, Sukhumvit Road,
Bangchack, Prakhonong, Bangkok 10260

Page 1 of 4

Equipment: Electronic Balance
Manufacturer: METTLER TOLEDO
Model: XSR205DU
Serial No.: C009071872
ID No.: UAE.WAO.012/2563
Order No.: 2402283
Operation No.: 2402283-001
Date of Receipt: 2 April 2024
Date of Calibration: 2 April 2024

Calibrated by Mr.Jerawut Prapawuttipong
Scientist
Approved by (Mr.Pheraphat Tuanjit)
Manager, Division of Calibration Laboratory
Responsible for the Technical Management Team
Date of Issue: 9 April 2024

The uncertainties are for a confidence probability of approximately 95%

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the National Food Institute.

F-CS-009 Revision: 01 Date: 20-04-65

Calibration Report

Certificate No.: 2402283-001-01
Equipment: Electronic Balance
Model: XSR205DU
Serial No.: C009071872
Capacity: 220 g
Manufacturer: METTLER TOLEDO
Resolution: 0.00001 g / 0.0001 g
ID No.: UAE.WAO.012/2563

Page 2 of 4

Date of Calibration: 2 April 2024
Environment Condition: Ambient Temperature: 24.5 ± 0.5 °C Relative Humidity: 47.5 ± 2.5 %

Place of Calibration: Laboratory, UNITED ANALYST AND ENGINEERING CONSULTANT CO., LTD.

Condition of Equipment: Good Condition

Condition of This Results of Calibration:

1. Calibration Method: NFI Method W-MA-001 In-House Method based on UKAS Lab 14 : 2019

2. Reference Standards:

Reference Standard	Model	Serial No.	Calibrated By	Certificate No.	Due Date
Standard Weight Class E2	1mg to 200g	8505567572	TCS	M23040535	8 April 2024
Instrument	Model	Serial No.	Calibrated By	Certificate No.	Due Date
Thermo-Hygro Meter	608-H1	NFI.BTH 016/23	Quality Reborn	QR24-0343	9 February 2025

3. This certification is traceable to SI UNIT

4. This certificate was certified only for the instrument we calibrated.

5. This result of calibration was found accurate as shown on date and place of calibration only.

Calibration Results:


1. Repeatability of Reading:

Nominal Value (g)	Standard Deviation of Reading (g)
40	0.000052
80	0.000063
100	0.000048
200	0.000053

2. Off-Center Error:

A mass of 100 g was placed and moved to various position on pan.

The balance reading obtained is given in the table.

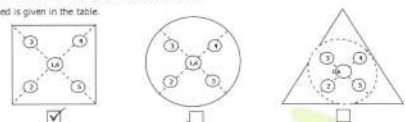

1	2	3	4	5	6	(Maximum Difference)
(g)	(g)	(g)	(g)	(g)	(g)	(g)
100.0002	100.0001	100.0002	99.9999	100.0001	100.0001	0.0003

F-CS-012 Revision: 01 Date: 20-04-65

Calibration Report

Certificate No.: 2402283-001-01
Equipment: Electronic Balance
Model: XSR205DU
Serial No.: C009071872
Capacity: 220 g
Manufacturer: METTLER TOLEDO
Resolution: 0.00001 g / 0.0001 g
ID No.: UAE.WAO.012/2563

Date of Calibration: 2 April 2024
Page 3 of 4

Calibration Results: (Continued)

Calibration Range: 0 - 80 g

Calibration Adjustment: Internal Calibration

3. Departure from Nominal Value: (Range: 0 - 80 g ; Resolution: 0.00001 g)

Nominal Value (g)	Standard Value (g)	Average Reading (g)	Correction (g)	Uncertainty (± g)	Coverage Factor
Unloaded	0.000000	0.000000	0.000000	0.0000088	2.00
0.001	0.001003	0.001011	-0.000008	0.0000091	2.00
0.005	0.005003	0.005009	-0.000006	0.0000094	2.00
0.01	0.010003	0.010000	0.000003	0.0000091	2.00
0.05	0.049996	0.050000	-0.000004	0.0000096	2.00
0.1	0.100011	0.100000	0.000011	0.000011	2.00
0.5	0.500016	0.500001	0.000015	0.000014	2.00
1	1.000003	1.000002	-0.000001	0.000016	2.00
2	2.000023	2.000001	0.000022	0.000017	2.00
5	5.000017	5.000002	0.000015	0.000020	2.00
10	10.000009	10.000000	0.000009	0.000026	2.00
20	20.000031	20.000002	0.000029	0.000037	2.00
30	30.000040	30.000003	0.000037	0.000052	2.00
50	50.000028	50.000004	0.000024	0.000068	2.00
80	80.000068	80.000005	0.000063	0.000111	2.00

F-CS-012 Revision: 01 Date: 20-04-65

Calibration Report

Certificate No.: 2402283-001-01
Equipment: Electronic Balance
Model: XSR205DU
Serial No.: C009071872
Capacity: 220 g
Manufacturer: METTLER TOLEDO
Resolution: 0.00001 g / 0.0001 g
ID No.: UAE.WAO.012/2563

Date of Calibration: 2 April 2024
Page 4 of 4

Calibration Results: (Continued)

Calibration Range: 81 - 200 g

Calibration Adjustment: Internal Calibration

3. Departure from Nominal Value: (Range: 81 - 200 g ; Resolution: 0.00001 g)

Nominal Value (g)	Standard Value (g)	Average Reading (g)	Correction (g)	Uncertainty (± g)	Coverage Factor
90	90.000010	90.000000	0.000010	0.000015	2.00
100	100.000006	100.000000	0.000006	0.000015	2.00
110	110.000007	110.000001	0.000006	0.000017	2.00
120	120.000009	120.000000	0.000009	0.000018	2.00
130	130.000018	130.000000	0.000018	0.000019	2.00
140	140.000014	140.000000	0.000014	0.000020	2.00
150	150.000009	150.000001	0.000008	0.000020	2.00
160	160.000016	160.000001	0.000015	0.000022	2.00
170	170.000012	170.000001	0.000011	0.000023	2.00
200	200.000016	200.000000	0.000016	0.000028	2.00

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k, providing a level of confidence of approximately 95 %.

F-CS-012 Revision: 01 Date: 20-04-65

Calibration Certificate

Certificate No.: 2502226-001-01
Client name: UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.
Address: 3 Soi Udomsuk 41, Sukhumvit Road,
Bangchack, Prakhnong, Bangkok 10260

Page 1 of 4

Equipment: Electronic Balance
Manufacturer: METTLER TOLEDO
Model: XSR205DU
Serial No.: C009071872
ID No.: UAE.WAO.012/2563
Order No.: 2502226
Operation No.: 2502226-001
Date of Receipt: 19 March 2025
Date of Calibration: 20 March 2025

Calibrated by Mr.Yothin Charoensuk
Scientist
Approved by *for N. Nijagubet*
(Mr.Pheraphat Tuanjit)
Manager, Division of Calibration Laboratory
Responsible for the Technical Management Team
Date of Issue: 25 March 2025

The uncertainties are for a confidence probability of approximately 95%

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the National Food Institute.

FCS-009 Revision: 01 Date: 20-04-65

2008 ปีที่ 35 ถนนสุขุมวิท 35 แขวงคลองเตย เขตคลองเตย กรุงเทพมหานคร 10110
2008 Soi 35, Anin Amani Road, Bang Yi Khan Subdistrict, Bang Phai District, Bangkok 10700, Thailand
Tel: +66(0) 21422 8508 Fax: +66(0) 21422 8545



เอกสารไม่ควบคุม

Calibration Report

Certificate No.: 2502226-001-01
Equipment: Electronic Balance
Manufacturer: METTLER TOLEDO
Model: XSR205DU
Serial No.: C009071872
Capacity: 82 g / 220 g
Resolution: 0.00001 g / 0.0001 g
ID No.: UAE.WAO.012/2563

Page 2 of 4

Date of Calibration: 20 March 2025

Environment Condition: Ambient Temperature: 21.2 ± 0.6 °C Relative Humidity: 48 ± 3.5 %

Place of Calibration: 208 Balance Room, UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.

Condition of Equipment: Good Condition

Condition of This Results of Calibration:

1. Calibration Method: NFI Method W-MA-001 In-House Method based on UKAS Lab 14 : 2019

2. Reference Standards:

Reference Standard	Model	Serial No.	Calibrated By	Certificate No.	Due Date
Standard Weight Class E2	1mg to 200g	8505567572	TCS	M24041005	19 April 2025
Instrument	Model	Serial No.	Calibrated By	Certificate No.	Due Date
Thermo-Hygro Meter	608-H1	NFL8TH 017/23	Quality Reborn	QR25-0542	10 February 2026

3. This certification is traceable to SI UNIT

4. This certificate was certified only for the instrument we calibrated.

5. This result of calibration was found accurate as shown on date and place of calibration only.

Calibration Results:


1. Repeatability of Reading:

Nominal Value (g)	Standard Deviation of Reading (g)
40	0.0000052
80	0.0000042
100	0.0000000
200	0.0000000

2. Off-Center Error:

A mass of 100 g was placed and moved to various position on pan.

The balance reading obtained is given in the table.



1	2	3	4	5	(Maximum Difference)
(g)	(g)	(g)	(g)	(g)	(g)
100.0001	100.0001	100.0001	100.0001	100.0001	0.0001

FCS-012 Revision: 01 Date: 20-04-65

2008 ปีที่ 35 ถนนสุขุมวิท 35 แขวงคลองเตย เขตคลองเตย กรุงเทพมหานคร 10110
2008 Soi 35, Anin Amani Road, Bang Yi Khan Subdistrict, Bang Phai District, Bangkok 10700, Thailand
Tel: +66(0) 21422 8508 Fax: +66(0) 21422 8545



เอกสารไม่ควบคุม

Calibration Report

Certificate No.: 2502226-001-01
Equipment: Electronic Balance
Manufacturer: METTLER TOLEDO
Model: XSR205DU
Serial No.: C009071872
Capacity: 82 g / 220 g
Resolution: 0.00001 g / 0.0001 g
ID No.: UAE.WAO.012/2563

Date of Calibration: 20 March 2025

Page 3 of 4

Calibration Results: (Continued)

Calibration Range: 0-80 g

Calibration Adjustment: Internal Calibration

3. Departure from Nominal Value: (Range: 0 - 82 g ; Resolution: 0.00001 g)

Nominal Value (g)	Standard Value (g)	Average Reading (g)	Correction (g)	Uncertainty (± g)	Coverage Factor k
Unload	0.000000	0.000000	0.000000	0.0000089	2.00
0.001	0.001003	0.001000	0.000000	0.0000092	2.00
0.005	0.005002	0.005000	0.000000	0.0000094	2.00
0.01	0.010003	0.010000	0.000000	0.0000091	2.00
0.05	0.049996	0.050000	0.000000	0.0000098	2.00
0.1	0.100011	0.100000	0.000011	0.000011	2.00
0.5	0.500016	0.500000	0.000016	0.000014	2.00
1	1.000003	1.000001	-0.000001	0.000016	2.00
2	2.000023	2.000005	-0.000018	0.000017	2.00
5	5.000015	5.000005	-0.000010	0.000021	2.00
10	10.000009	10.000005	-0.000004	0.000026	2.00
20	20.000030	20.000012	-0.000018	0.000037	2.00
30	30.000039	30.000012	-0.000027	0.000050	2.00
50	50.000028	50.000014	-0.000014	0.000068	2.00
80	80.000067	80.000020	-0.000047	0.00011	2.00

Calibration Report

Certificate No.: 2502226-001-01
Equipment: Electronic Balance
Manufacturer: METTLER TOLEDO
Model: XSR205DU
Serial No.: C009071872
Capacity: 82 g / 220 g
Resolution: 0.00001 g / 0.0001 g
ID No.: UAE.WAO.012/2563

Date of Calibration: 20 March 2025

Page 4 of 4

Calibration Results: (Continued)

Calibration Range: >80-200 g

Calibration Adjustment: Internal Calibration

3. Departure from Nominal Value: (Range: >80 - 200 g ; Resolution: 0.00001 g)

Nominal Value (g)	Standard Value (g)	Average Reading (g)	Correction (g)	Uncertainty (± g)	Coverage Factor k
90	90.000010	90.00002	-0.00001	0.000015	2.00
100	100.000006	100.00001	0.00000	0.000016	2.00
110	110.000007	110.00001	0.00000	0.000017	2.00
120	120.000009	120.00002	-0.00001	0.000018	2.00
130	130.000010	130.00002	-0.00001	0.000019	2.00
140	140.000013	140.00002	-0.00001	0.000019	2.00
150	150.000009	150.00002	-0.00001	0.000021	2.00
160	160.000010	160.00002	-0.00001	0.000022	2.00
170	170.000012	170.00002	-0.00001	0.000023	2.00
200	200.000013	200.00002	-0.00001	0.000028	2.00

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k ; providing a level of confidence of approximately 95 %.

----- End -----

FCS-012 Revision: 01 Date: 20-04-65

2008 ปีที่ 35 ถนนสุขุมวิท 35 แขวงคลองเตย เขตคลองเตย กรุงเทพมหานคร 10110
2008 Soi 35, Anin Amani Road, Bang Yi Khan Subdistrict, Bang Phai District, Bangkok 10700, Thailand
Tel: +66(0) 21422 8508 Fax: +66(0) 21422 8545



เอกสารไม่ควบคุม

FCS-012 Revision: 01 Date: 20-04-65

2008 ปีที่ 35 ถนนสุขุมวิท 35 แขวงคลองเตย เขตคลองเตย กรุงเทพมหานคร 10110
2008 Soi 35, Anin Amani Road, Bang Yi Khan Subdistrict, Bang Phai District, Bangkok 10700, Thailand
Tel: +66(0) 21422 8508 Fax: +66(0) 21422 8545



เอกสารไม่ควบคุม



Certificate of Calibration

Cert. No.: 24TM1113
Page : 1 of 3

Equipment : BOD Incubator
Manufacturer : ARCO
Model : UC4-1320
Serial No. : -
ID No. : UAE.WAO.002/2550
Submitted by : United Analyst and Engineering Consultant Co.,Ltd.
3 Soi Udomsuk 41, Sukhumvit Road,
Bangchak, Phrakhanong,
Bangkok 10260
Location : Lab Floor 2
Received Order : 11 July 2024
Calibration Date : 11 July 2024
Ambient Temperature : $(26 \pm 10) ^\circ\text{C}$
Relative Humidity : $(50 \pm 30) \%$
Calibrated by : Tawatchai Pama
Approved by :
() Ponpan Palpim
(✓) Suwit Imjai
() Kunchit Promprat
Issue Date : 14 July 2024

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

เอกสารไม่ควบคุม



Equipment : BOD Incubator
Condition As-Received : Used Item
Reference : 2407-0243OC-1
Procedure Used :-

Cert. No.: 24TM1113
Page : 2 of 3

Calibration were conducted using calibration procedure CP-OT02 based on TLAS G-20 according to direct measurement method with Data Acquisition which connected with Resistance Temperature Detector (RTD).
The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

Instrument	Serial No.	Cert. No.	Traceable	Due Date
1) Data Acquisition	MY49023932	23LM122	TPA	26 Jul 2024

2. This certificate is valid only to the item calibrated on date and place of calibration.
3. This certification is traceable to the International System of Unit.


Remark : TPA : Technology Promotion Association (Thailand - Japan)

Result of Calibration :- (*) Without Adjustment

Function of UUC* : Temperature Source

Fresh air setting : Not Available

Environment during calibration		
	Beginning	Finished
Temp. (°C)	29	32
REL.Humid. (%)	78	85
AC Supply (Volt)	233	234



Probe Installation Details :

a =	10	cm
b =	10	cm
c =	10	cm

Dimension of Chamber :

D =	0.62	m
W =	1.2	m
H =	1.2	m
Capacity =	0.89	m ³

Position :	Ref. Std. ID No.:
1	19-16RTD-01
2	19-16RTD-02
3	19-16RTD-03
4	19-16RTD-04
5	19-16RTD-05
6	19-16RTD-06
7	21-16RTD-07
8	19-16RTD-08
9 (ref.)	19-16RTD-09

Certificate of Calibration

Cert. No.: 24TM1114
Page : 1 of 3



Equipment : BOD Incubator
Condition As-Received : Used Item
Reference : 2407-0243OC-1
Result of Calibration :- (*) Without Adjustment
Function of UUC* : Temperature Source
Fresh air setting : Not Available

Cert. No.: 24TM1113
Page : 3 of 3

Calibration Point (°C)	UUC* Setting (°C)	UUC* Reading (°C)	Temperature stability (± °C)	Temperature uniformity (°C)	Overall Variation (°C)	Coverage Factor <i>k</i>
20.0	20.0	19.8	0.55	0.66	1.5	2

Calibration Point (°C)	Measured Temperature (°C)									Uncertainty (± °C)
	1	2	3	4	5	6	7	8	9 (ref.)	
20.0	20.210	20.331	20.162	19.645	20.287	20.070	19.838	19.781	19.954	0.79

Average* : The average of 30 values in each position.

Temperature stability : One-half of the greatest maximum difference of measured temperature at any one sensor.

Temperature uniformity : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.

Overall Variation : The Difference of the maximum and minimum measured temperatures throughout observation.

UUC* : Unit Under Calibration

Note : The reported uncertainty of measurement was included stability and excluded uniformity .

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-000-



Certificate of Calibration

Cert. No.: 24TM1114
Page : 1 of 3

Equipment : BOD Incubator
Manufacturer : ARCO
Model : UC4-1320
Serial No. : -
ID No. : UAE.WAO.018/2559
Submitted by : United Analyst and Engineering Consultant Co.,Ltd.
3 Soi Udomsuk 41, Sukhumvit Road,
Bangchak, Phrakhanong,
Bangkok 10260
Location : Lab Floor 2
Received Order : 11 July 2024
Calibration Date : 11 July 2024
Ambient Temperature : $(26 \pm 10) ^\circ\text{C}$
Relative Humidity : $(50 \pm 30) \%$
Calibrated by : Tawatchai Pama
Approved by :
() Ponpan Palpim
(✓) Suwit Imjai
() Kunchit Promprat
Issue Date : 14 July 2024

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

เอกสารไม่ควบคุม

เอกสารไม่ควบคุม



Equipment : BOD Incubator
Condition As-Received : Used Item
Reference : 2407-0243OC-2

Cert. No.: 24TM1114
Page : 2 of 3

Procedure Used :-

Calibration were conducted using calibration procedure CP-OT02 based on TLAS G-20 according to direct measurement method with Data Acquisition which connected with Resistance Temperature Detector (RTD).

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

Instrument	Serial No.	Cert. No.	Traceable	Due Date
1) Data Acquisition	MY49023932	23LM122	TPA	26 Jul 2024

2. This certificate is valid only to the item calibrated on date and place of calibration.


3. This certification is traceable to the International System of Unit.

Remark : TPA : Technology Promotion Association (Thailand - Japan)

Result of Calibration :- (*) Without Adjustment

Function of UUC* : Temperature Source

Fresh air setting : Not Available



Environment during calibration		
	Beginning	Finished
Temp. (°C)	29	29
REL.Humid. (%)	78	72
AC Supply (Volt)	233	234

Position :	Ref. Std. ID No.:
1	20-16RTD-10
2	20-16RTD-02
3	20-16RTD-03
4	23-16RTD-04
5	22-16RTD-05
6	20-16RTD-06
7	20-16RTD-07
8	22-16RTD-08
9 (ref.)	22-16RTD-09

Probe Installation Details :

a = 10 cm
b = 10 cm
c = 10 cm

Dimension of Chamber :

D = 0.62 m
W = 1.2 m
H = 1.2 m
Capacity = 0.89 m³



Equipment : BOD Incubator
Condition As-Received : Used Item
Reference : 2407-0243OC-2
Result of Calibration :- (*) Without Adjustment
Function of UUC* : Temperature Source
Fresh air setting : Not Available

Cert. No.: 24TM1114
Page : 3 of 3

Calibration Point (°C)	UUC* Setting (°C)	UUC* Reading (°C)	Temperature stability (± °C)	Temperature uniformity (°C)	Overall Variation (°C)	Coverage Factor k
20.0	20.0	19.9	0.29	0.81	1.2	2

Calibration Point (°C)	Measured Temperature (°C)									Uncertainty (± °C)
	Position									
	1	2	3	4	5	6	7	8	9 (ref.)	
20.0	20.361	19.640	20.312	20.079	19.908	19.872	19.955	19.818	19.758	0.48

Average* : The average of 30 values in each position.

Temperature stability : One-half of the greatest maximum difference of measured temperature at any one sensor.

Temperature uniformity : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.

Overall Variation : The Difference of the maximum and minimum measured temperatures throughout observation.

UUC* : Unit Under Calibration

Note : The reported uncertainty of measurement was included stability and excluded uniformity .

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

เอกสารไม่ควบคุม

เอกสารไม่ควบคุม



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000-29 FAX. 0-2719-9484



Cert. No.: 24TM588
Page : 1 of 3

Certificate of Calibration

Equipment : BOD Incubator
Manufacturer : ARCO
Model : UR-1320
Serial No. : -
ID No. : UAE.WAO.006/2553
Submitted by : United Analyst and Engineering Consultant Co.,Ltd.
3 Soi Udomsuk 41, Sukhumvit Road,
Bangchak, Phrakhanong,
Bangkok 10260
Location : Lab Floor 2
Received Order : 01 April 2024
Calibration Date : 01 April 2024
Ambient Temperature : (26 ± 10) °C
Relative Humidity : (50 ± 30) %
Calibrated by : Krisda Malee
Approved by :
() Ponpan Paipim
(✓) Suwit Imjai
() Kunchit Promprat

Issue Date : 5 April 2024

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

เอกสารไม่ควบคุม

A 0065064



Equipment : BOD Incubator
Condition As-Received : Used Item
Reference : 2404-0004OC-2

Cert. No.: 24TM588
Page : 2 of 3

Procedure Used :-

Calibration were conducted using calibration procedure CP-OT02 based on TLAS G-20 according to direct measurement method with Data Acquisition which connected with Resistance Temperature Detector (RTD).

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

Instrument	Serial No.	Cert. No.	Traceable	Due Date
1) Data Acquisition	MY57013711	23LM115	TPA	11 Jul 2024

2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certification is traceable to the International System of Unit.


Remark : TPA : Technology Promotion Association (Thailand - Japan)

Result of Calibration :- (*) Without Adjustment

Function of UUC* : Temperature Source

Fresh air setting : Not Available

Environment during calibration		
	Beginning	Finished
Temp. (°C)	28	27
REL.Humid. (%)	45	47
AC Supply (Volt)	220	221



Probe Installation Details :

a = 10 cm
b = 10 cm
c = 10 cm

Dimension of Chamber :

D = 0.62 m
W = 1.2 m
H = 1.2 m
Capacity = 0.89 m³

Position :	Ref. Std. ID No.:
1	22-18RTD-2/1
2	18RTD-2/2
3	18RTD-2/3
4	18RTD-2/4
5	18RTD-2/5
6	18RTD-2/6
7	18RTD-2/7
8	18RTD-2/8
9 (ref.)	18RTD-2/9

เอกสารไม่ควบคุม

a 1209741



Equipment : BOD Incubator
 Condition As-Received : Used Item
 Reference : 2404-0004OC-2
 Result of Calibration :- (*) Without Adjustment
 Function of UUC* : Temperature Source
 Fresh air setting : Not Available

Cert. No.: 24TM588
 Page : 3 of 3

Calibration Point (°C)	UUC* Setting (°C)	UUC* Reading (°C)	Temperature stability (± °C)	Temperature uniformity (°C)	Overall Variation (°C)	Coverage Factor k
20.0	20.0	19.9	0.47	0.69	1.4	2

Calibration Point (°C)	Measured Temperature (°C)									Uncertainty (± °C)
	1	2	3	4	5	6	7	8	9 (ref.)	
20.0	20.289	19.835	20.129	19.985	20.190	20.180	20.300	20.457	20.248	0.67

Average* : The average of 30 values in each position.

Temperature stability : One-half of the greatest maximum difference of measured temperature at any one sensor.

Temperature uniformity : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.

Overall Variation : The Difference of the maximum and minimum measured temperatures throughout observation.

UUC* : Unit Under Calibration

Note : The reported uncertainty of measurement was included stability and excluded uniformity.

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-000-

เอกสารไม่ควบคุม

a 1209740

Technology



Service Report

TO	FOR
Company: United Analyst and Engineering Consultant Co., Ltd. _ Bangkok-HQ	Work Order Number: WO-00018067
Address: 700/2 หมู่ที่ 1 Phrakhanong District, Bangkok, 10260	Contact: Kamphong Boonpuang
	Email: kamphong.b@uaeconsultant.co.th
	Tel: +66 2763 2828 (7021), +66 8 6347 7390

WORK ORDER INFORMATION			
Top-Level		Order Type	Preventive Maintenance
Installed Product ID	IB-00105024	Billing Type	Paid
Product	SKALAR SAN++ Classic 2SAN59000	PO No.	SSPR2400629
Serial No.	182688	Warranty No.	
		Contract No.	

PRODUCTS SERVICED		
Installed Product Id	Serial Number	Product

PROBLEM DESCRIPTION	
PM 1/1	

Line Number	Engineer	Start Date And Time	End Date And Time	Billable Labor Hour	Billable Travel Hour	Travel KM
WL-00071161	Yongyuth Chanphong	02/20/2024 8:53 AM	02/20/2024 6:07 PM	9.23333		
WL-00092966	Ronnarit Dechnawarat	02/20/2024 8:53 AM	02/20/2024 6:07 PM	9.23333		
Total				18.46666	0	0

กำหนดจุดห้ามใช้งาน

References Certificate Number. : 234TM588

Equipment : BOD Incubator

Model : UR-1320


Serial No. : -

ID No. : UAE.WAO.006/2553

Manufacturer : ARCO

Calibration Point : 20.0 °C

Unit Under Calibration Setting : 20.0 °C

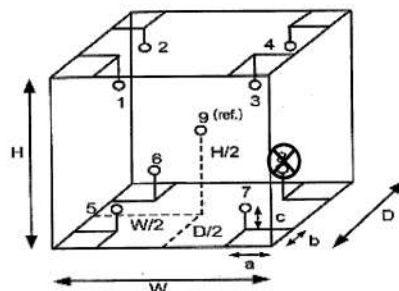

รูปภาพเครื่องมือ แสดงจุดที่ได้รับการสอบเทียบ และสัญลักษณ์ ⊗ แสดงจุดห้ามใช้งาน

กำหนดจุดห้ามใช้งานตำแหน่งที่...8.....

หมายเหตุ เก็บใบแนบ.....

! Reach us at DKSH Service-Hotline : +66 2 639 7000 2533 Sukhumvit Road, Bangkok, 10260, Phrakhanong, Bangkok, Thailand Phone +66 2 639 7000 Fax +66 2 333 1026

เอกสารไม่ควบคุม

Technology



Line Number	Work Description
WL-00071161	ทำ PM เรียบร้อย
WL-00092966	ทำ PM เรียบร้อย

PARTS CONSUMED		
Part No	Part Description	Quantity

EXPENSES			
Part No	Expense Type	Description	Line Quantity

RECOMMENDED PARTS	
แนะนำอะไหล่ที่ต้องสั่งซื้อเพิ่มเติมดังนี้ , อะไหล่ พารามิเตอร์ Ammonia จำนวน 2 รายการ (9220, 3026) , อะไหล่ พารามิเตอร์ Phenol และ Cyanide จำนวน 6 รายการ (5454, 3028, 3031, 3034, 3036, 3150)	

REMARKS

Travel Time Disclaimer:

Please note that the travel time in this report only includes time taken to reach the installed equipment location. It does not include our engineer's return travel time.

Customer Signature:

Kamphong b

Customer Signature

Technician: Yongyuth Chanphong
 Job Title: Service Manager
 Email: yongyuth.yc@dksh.com

Date: 04/10/2024

Test Report

Customers	United Analyst and Engineering Consultant Co., Ltd.		
Equipment	Continuous Flow Analyzer	Manufacturer	SKALAR
Controller Mdel	SA5000	Auto Sample Model	SA1052
Controller Serial No.	182688	Auto Sample Serial No.	181729
Date of test	20-Feb-2024	Period	12 Month
Environment temperature	24.7 °C	Humidity	62.2 %RH

Results

Instrument Checked	

Item	Characteristic	Before	After	Remark
1	Visual inspect	<input type="checkbox"/> Pass <input type="checkbox"/> Fail	<input type="checkbox"/> Pass <input type="checkbox"/> Fail	
2	Power supply (210 - 240 VAC)	220 VAC	220 VAC	
3	Computer	<input type="checkbox"/> Pass <input type="checkbox"/> Fail	<input type="checkbox"/> Pass <input type="checkbox"/> Fail	
4	Program	<input type="checkbox"/> Pass <input type="checkbox"/> Fail	<input type="checkbox"/> Pass <input type="checkbox"/> Fail	
5	Auto sampler	<input type="checkbox"/> Pass <input type="checkbox"/> Fail	<input type="checkbox"/> Pass <input type="checkbox"/> Fail	
6	Module holder			
	- Motor pump	<input type="checkbox"/> Pass <input type="checkbox"/> Fail	<input type="checkbox"/> Pass <input type="checkbox"/> Fail	
	- Pump tube	<input type="checkbox"/> Pass <input type="checkbox"/> Fail	<input type="checkbox"/> Pass <input type="checkbox"/> Fail	+
	- Air-injection	<input type="checkbox"/> Pass <input type="checkbox"/> Fail	<input type="checkbox"/> Pass <input type="checkbox"/> Fail	*
	- Chemistry manifolds, Switching valve, Coil, Membrane	<input type="checkbox"/> Pass <input type="checkbox"/> Fail	<input type="checkbox"/> Pass <input type="checkbox"/> Fail	**,***
7	Detector			
	- Filter	<input type="checkbox"/> Pass <input type="checkbox"/> Fail	<input type="checkbox"/> Pass <input type="checkbox"/> Fail	
	- Flow cell	<input type="checkbox"/> Pass <input type="checkbox"/> Fail	<input type="checkbox"/> Pass <input type="checkbox"/> Fail	
	- Lamp	<input type="checkbox"/> Pass <input type="checkbox"/> Fail	<input type="checkbox"/> Pass <input type="checkbox"/> Fail	
8	Interface	<input type="checkbox"/> Pass <input type="checkbox"/> Fail	<input type="checkbox"/> Pass <input type="checkbox"/> Fail	
9	Rinsing valves	<input type="checkbox"/> Pass <input type="checkbox"/> Fail <input type="checkbox"/> N/A	<input type="checkbox"/> Pass <input type="checkbox"/> Fail <input type="checkbox"/> N/A	
10	Temperature / Reactor	<input type="checkbox"/> Pass <input type="checkbox"/> Fail <input type="checkbox"/> N/A	<input type="checkbox"/> Pass <input type="checkbox"/> Fail <input type="checkbox"/> N/A	
11	Flame photometer	<input type="checkbox"/> Pass <input type="checkbox"/> Fail <input type="checkbox"/> N/A	<input type="checkbox"/> Pass <input type="checkbox"/> Fail <input type="checkbox"/> N/A	
12	UPS / Stabilizer	<input type="checkbox"/> Pass <input type="checkbox"/> Fail <input type="checkbox"/> N/A	<input type="checkbox"/> Pass <input type="checkbox"/> Fail <input type="checkbox"/> N/A	

Warning and Error Checked

Item	Event	Before	After
13	Error list	<input type="checkbox"/> None <input type="checkbox"/> Appear : _____ _____ _____	<input type="checkbox"/> None <input type="checkbox"/> Appear : _____ _____ _____

Check with Standard

Item	Characteristic	Before	After	Remark
14	Base Line Test	<input type="checkbox"/> Pass <input type="checkbox"/> Fail <input type="checkbox"/> N/A	<input type="checkbox"/> Pass <input type="checkbox"/> Fail <input type="checkbox"/> N/A	
15	Detector Signal Test	<input type="checkbox"/> Pass <input type="checkbox"/> Fail <input type="checkbox"/> N/A	<input type="checkbox"/> Pass <input type="checkbox"/> Fail <input type="checkbox"/> N/A	

Summary of checked

- ☐ The instrument can work normally and efficiently. (เครื่องมือวัดสามารถทำงานได้ปกติและมีประสิทธิภาพ)
- ☐ The instrument can work but it's requiring maintenance. (เครื่องมือวัดสามารถทำงานได้แต่ต้องบำรุงรักษา)
- ☐ The instrument could not work it's requiring to repair. (เครื่องมือวัดไม่สามารถทำงานได้แต่ต้องการซ่อมบำรุง)

Remark :

- * Pump tube และ Air tube เริ่มเสื่อมสภาพ ได้เปลี่ยนอะไหล่ทั้งหมดแล้วตามระยะการใช้งาน

Standard Equipment Used



Equipment	Equipment I.D.
Digital multi meter	S/N 57600592 Due date : 8-Jul-2024
Thermo hygrometer	S/N 39520444 Due date : 27-Dec-2024



Test By : _____
(Mr. Yongyuth Chanphong)

Approved by : _____
(Mr. Eknopong Wankliang)

Position : Supervisor, Technical Service

Position : Manager, Technical Services

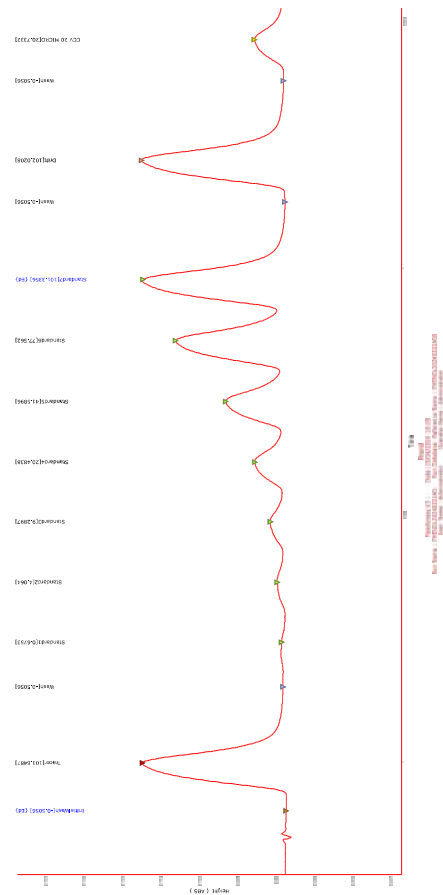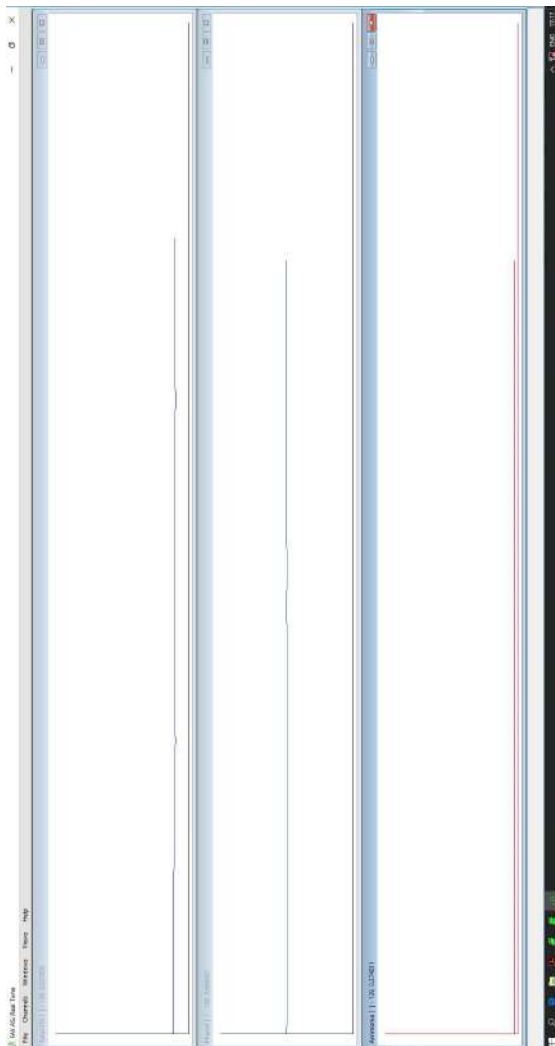

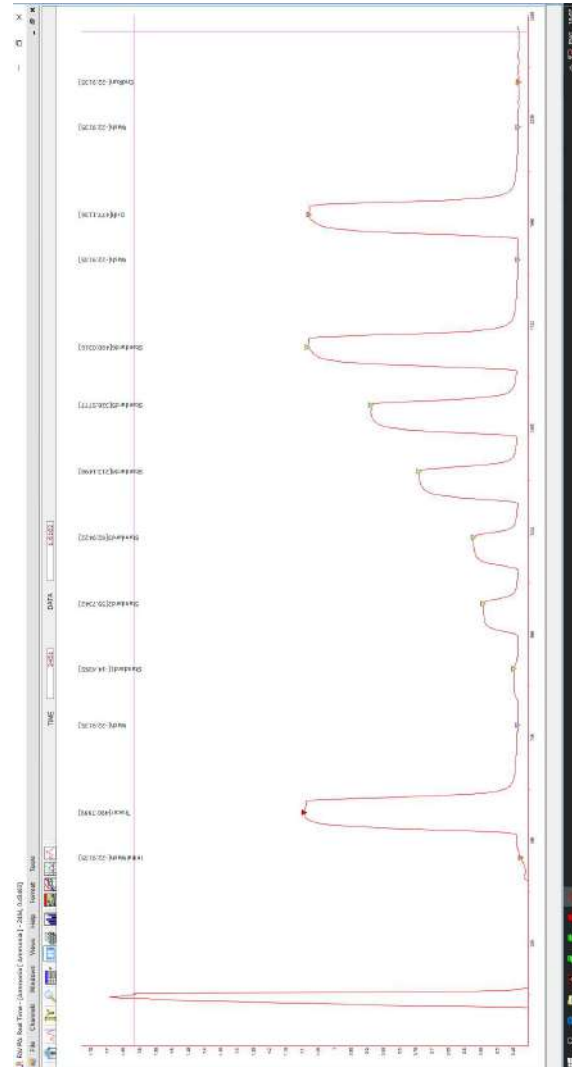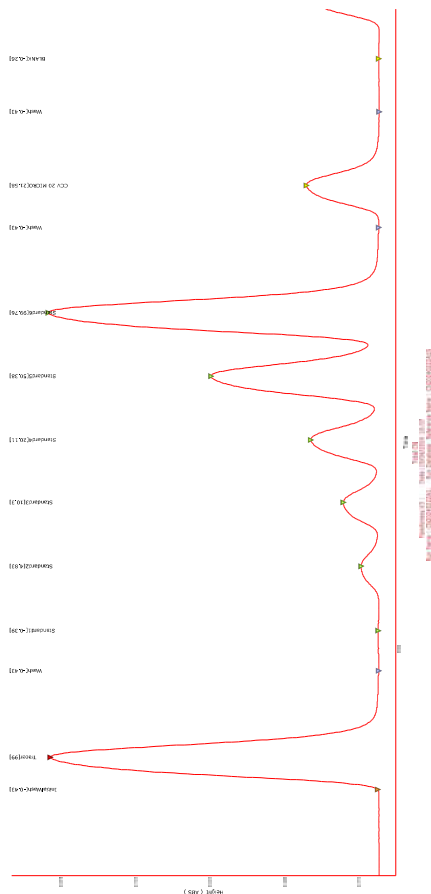

Technology



Service Report

TO	FOR
Company: United Analyst and Engineering Consultant Co., Ltd., Bangkok+HQ Address: 700/2 หมู่ที่ 1 Phrakhanong District, Bangkok, 10260	Work Order Number: WO-00074079 Contact: Karnphong Boonpuang Email: karnphong.b@uaeconsultant.co.th Tel: +66 2763 2828 (7021), +66 8 6347 7390

WORK ORDER INFORMATION			
Top-Level		Order Type	Preventive Maintenance
Installed Product ID	IB-00105024	Billing Type	Chargeable
Product	SKALAR 2SAN59000 SAN++ Classic CFA 230V 2SAN59000	PO No.	HPO-250400209
Serial No.	182688	Warranty No.	
		Contract No.	

PRODUCTS SERVICED		
Installed Product Id	Serial Number	Product
IB-00105024	182688	SKALAR 2SAN59000 SAN++ Classic CFA 230V 2SAN59000

PROBLEM DESCRIPTION	
PM 1 ครั้ง/ปี **ใบเสนอราคาเลขที่ Q-120095	

Line Number	Engineer	Start Date And Time	End Date And Time	Billable Labor Hour	Billable Travel Hour	Travel KM
WL-00342192	Yongyuth Chanphong	05/23/2025 9:30 AM	05/23/2025 6:00 PM	8.5		
Total				8.5	0	0

! Reach us at DKSH Service-Hotline : +66 2 639 7000
2533 Sukhumvit Road, Bangkok, 10260, Phrakhanong, Bangkok, Thailand
Phone +66 2 639 7000 Fax +66 2 333 1026

Delivering Growth - in Asia and beyond

เอกสารไม่ควบคุม Page 1 of 2

Technology



Line Number	Work Description
WL-00342192	- ทำ PM เสร็จแล้ว, เครื่องพร้อมใช้งาน

PARTS CONSUMED		
Part No	Part Description	Quantity

EXPENSES			
Part No	Expense Type	Description	Line Quantity

RECOMMENDED PARTS	
อะไหล่สำรองที่ควรซื้อทั้งหมด 7 รายการ คือ Pump tube 3 รายการ (SA3028, SA3032 และ SA3034), หลอดไฟ Halogen 6V/10W (90020012) 1 รายการ จำนวน 2 หลอด, Tubing polyethylene 3 รายการ (SA3142, SA5141 และ SA5142)	

REMARKS

Travel Time Disclaimer:
Please note that the travel time in this report only includes time taken to reach the installed equipment location. It does not include our engineer's return travel time.

Customer Signature:	Technician: Yongyuth Chanphong Job Title: Service Manager Email: yongyuth.yc@dksh.com
Customer Signature	
Date: 06/06/2025	

! Reach us at DKSH Service-Hotline : +66 2 639 7000
2533 Sukhumvit Road, Bangkok, 10260, Phrakhanong, Bangkok, Thailand
Phone +66 2 639 7000 Fax +66 2 333 1026

Delivering Growth - in Asia and beyond

เอกสารไม่ควบคุม Page 2 of 2

Test Report			
Job No. WO-00074079			
Customers	United Analyst and Engineering Consultant Co., Ltd.		
Equipment	Continuous Flow Analyzer	Manufacturer	SKALAR
Controller Mdel	SA5000	Auto Sample Model	SA1052
Controller Serial No.	182688	Auto Sample Serial No.	181729
Date of test	23-May-2025	Period	12 Month
Environment temperature	24.3 °C	Humidity	54.4 %RH

Results

Item	Characteristic	Before		After		Remark
1	Visual inspect	<input checked="" type="checkbox"/> Pass	<input type="checkbox"/> Fail	<input checked="" type="checkbox"/> Pass	<input type="checkbox"/> Fail	
2	Power supply (210 - 240 VAC)	220	VAC	220	VAC	
3	Computer	<input checked="" type="checkbox"/> Pass	<input type="checkbox"/> Fail	<input checked="" type="checkbox"/> Pass	<input type="checkbox"/> Fail	
4	Program	<input checked="" type="checkbox"/> Pass	<input type="checkbox"/> Fail	<input checked="" type="checkbox"/> Pass	<input type="checkbox"/> Fail	
5	Auto sampler	<input checked="" type="checkbox"/> Pass	<input type="checkbox"/> Fail	<input checked="" type="checkbox"/> Pass	<input type="checkbox"/> Fail	
6	Module holder					
	- Motor pump	<input checked="" type="checkbox"/> Pass	<input type="checkbox"/> Fail	<input checked="" type="checkbox"/> Pass	<input type="checkbox"/> Fail	
	- Pump tube	<input type="checkbox"/> Pass	<input type="checkbox"/> Fail	<input checked="" type="checkbox"/> Pass	<input type="checkbox"/> Fail	*
	- Air-injection	<input checked="" type="checkbox"/> Pass	<input type="checkbox"/> Fail	<input checked="" type="checkbox"/> Pass	<input type="checkbox"/> Fail	*
	- Chemistry manifolds, Switching valve, Coil, Membrane	<input checked="" type="checkbox"/> Pass	<input type="checkbox"/> Fail	<input checked="" type="checkbox"/> Pass	<input type="checkbox"/> Fail	
7	Detector					
	- Filter	<input checked="" type="checkbox"/> Pass	<input type="checkbox"/> Fail	<input checked="" type="checkbox"/> Pass	<input type="checkbox"/> Fail	
	- Flow cell	<input checked="" type="checkbox"/> Pass	<input type="checkbox"/> Fail	<input checked="" type="checkbox"/> Pass	<input type="checkbox"/> Fail	
	- Lamp	<input checked="" type="checkbox"/> Pass	<input type="checkbox"/> Fail	<input checked="" type="checkbox"/> Pass	<input type="checkbox"/> Fail	
8	Interface	<input checked="" type="checkbox"/> Pass	<input type="checkbox"/> Fail	<input checked="" type="checkbox"/> Pass	<input type="checkbox"/> Fail	
9	Rinsing valves	<input checked="" type="checkbox"/> Pass	<input type="checkbox"/> Fail	<input checked="" type="checkbox"/> Pass	<input type="checkbox"/> Fail	N/A
10	Temperature / Reactor	<input checked="" type="checkbox"/> Pass	<input type="checkbox"/> Fail	<input checked="" type="checkbox"/> Pass	<input type="checkbox"/> Fail	N/A
11	Flame photometer	<input checked="" type="checkbox"/> Pass	<input type="checkbox"/> Fail	<input checked="" type="checkbox"/> Pass	<input type="checkbox"/> Fail	N/A
12	UPS / Stabilizer	<input checked="" type="checkbox"/> Pass	<input type="checkbox"/> Fail	<input checked="" type="checkbox"/> Pass	<input type="checkbox"/> Fail	N/A

Warning and Error Checked

Item	Event	Before	After
13	Error list	<input type="checkbox"/> None <input type="checkbox"/> Appear : _____	<input type="checkbox"/> None <input type="checkbox"/> Appear : _____

Check with Standard

Item	Characteristic	Before			After			Remark
14	Base Line Test	<input type="checkbox"/> Pass	<input type="checkbox"/> Fail	<input type="checkbox"/> N/A	<input checked="" type="checkbox"/> Pass	<input type="checkbox"/> Fail	<input type="checkbox"/> N/A	
15	Detector Signal Test	<input type="checkbox"/> Pass	<input type="checkbox"/> Fail	<input type="checkbox"/> N/A	<input checked="" type="checkbox"/> Pass	<input type="checkbox"/> Fail	<input type="checkbox"/> N/A	

Summary of checked

- ☒ The instrument can work normally and efficiently. (เครื่องมือสามารถทำงานได้ปกติและประสิทธิภาพ)
- ☐ The instrument can work but it's requiring to maintenance. (เครื่องมือสามารถทำงานได้แต่ต้องบำรุงรักษา)
- ☐ The instrument could not work it's requiring to repair. (เครื่องมือทำงานไม่ได้ต้องมีการซ่อมบำรุง)

Remark :

* Pump tube, Tubing polyethylene and Air tube เป็นอะไหล่เก่า ไม่เป็นอะไหล่ใหม่ตามข้อกำหนดการใช้งาน

- หมายเหตุ และระยะเวลาในการสอบเทียบ 7 รายการ ดังนี้
- อะไหล่ พาร์ตของ Ammonia จำนวน 3 รายการ (SA3032, SA5141 และ 90020012)
 - อะไหล่ พาร์ตของ Phenol and Cyanide จำนวน 6 รายการ (SA3028, SA3034, SA3142, SA5142 และ 90020012)

Standard Equipment Used

Equipment	Equipment I.D.	
Digital multi meter	S/N 57600592	Due date : 19-Jun-2025
Thermo hygrometer	S/N 39520444/904	Due date : 27-Dec-2025

Test By : 
(Mr. Yongyuth Chanphong)

Approved by : 
(Mr. Eknaphong Wankiang)



Position : Supervisor, Technical Service

Position : Manager, Technical Services

Base Line Test : Reagent_Baseline_CN_Phenol_NH3





Detector Signal Test : Phenol

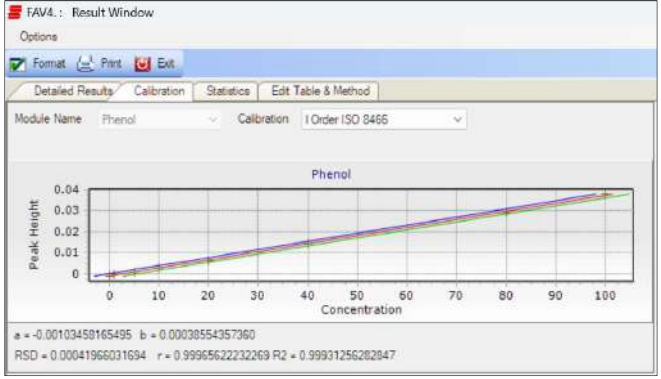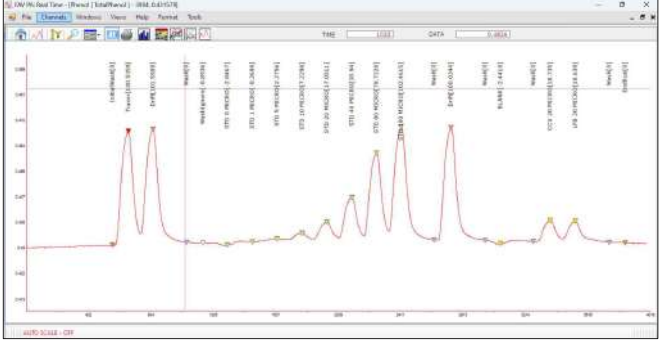



Detector Signal Test : NH3

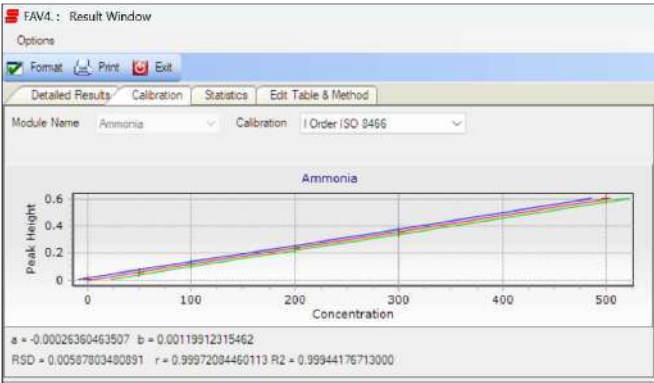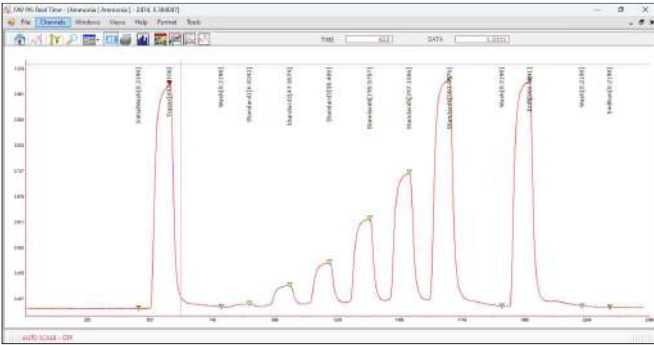

DKSH Technology Limited (Head office)
2533 Sukhumvit Road, Bangkok, Phrakhanong, Bangkok, 10260
Phone +66 2 639 7000, Mobile +66 93 813 8681, yongyuth-yc@dksh.com, www.dksh.com



Delivering Growth – in Asia and Beyond

เอกสารไม่ควบคุม

Page 5/2



Detector Signal Test : CN

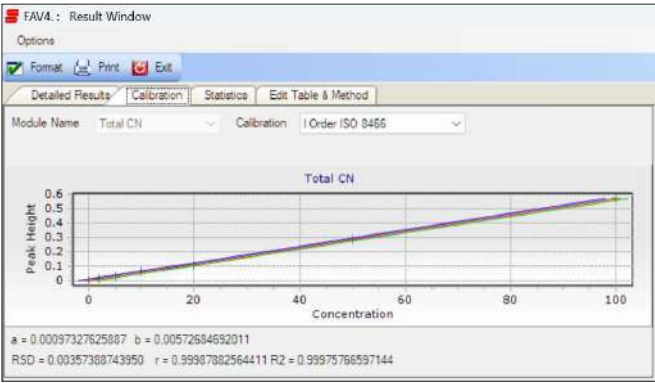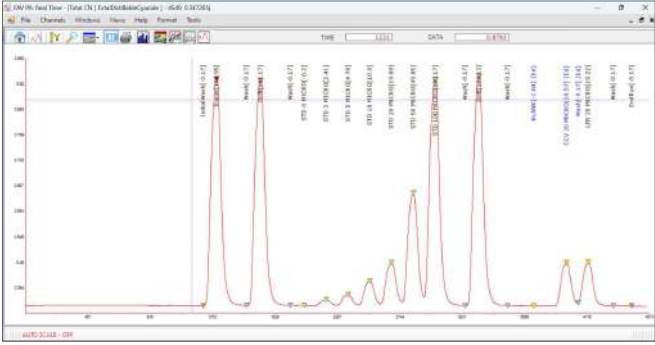

DKSH Technology Limited (Head office)
2533 Sukhumvit Road, Bangkok, Phrakhanong, Bangkok, 10260
Phone +66 2 639 7000, Mobile +66 93 813 8681, yongyuth-yc@dksh.com, www.dksh.com

Delivering Growth – in Asia and Beyond

เอกสารไม่ควบคุม

Page 6/2



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3 : EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL: 0-2717-3000 FAX: 0-2719-9484

Certificate of Testing

Cert.No.: 24TW271
Page.: 1 of 2

Equipment : DO Meter
Manufacturer : Horiba
Model : LAQUA-DO210
Serial No. : HE9M0013
ID No. : UAE.EFM.016/2563 (EFM.DO.05/63)
Received Date : 24 December 2024
Test Date : 25 December 2024
Reference : 2412-0604WSC-1
Submitted by : United Analyst and Engineering Consultant Co.,Ltd.
3 Soi Udomsuk 41, Sukhumvit Road,
Bangchak, Phrakhanong, Bangkok 10260
Laboratory Condition : Temperature (25 ± 5) °C
Humidity (50 ± 20) %
Test Procedure : In - house method : CP-CH9
by Comparison Technique with Azide Modification Method
Tested by : Walailak Sirithean
Approved by :
Approved Signatory
() Pornthippa Tameyakul
() Ponpan Palpim
(✓) Saithip Meangmai
Issue Date : 25 December 2024



Cert.No.: 24TW271
Page.: 2 of 2

Condition of this result of calibration

1. Reference Standard Instruments :
This certification is traceable to the International System of Unit through the reference standards
Laboratory of Industrial Calibration Center, Technology Promotion Association (Thailand-Japan).

Instruments	Serial No.	ID No.	Certificate No.	Due Date
1. Burette	-	130BU10	23CG1172	22 Mar 2025
2. Balance	14233821	110RC001	24MM131	04 July 2025

Material	Manufacturer	Lot.No.	Assay
Sodium Thiosulfate 5-Hydrate AR	KEMAUS	Z203162447	99.6%

Result : Dissolved Oxygen Meter Adjustment With Air 100 %
Dissolved Oxygen Probe No.: 9K9G0097

Titration Method (Azide Modification Method)	DO Meter Reading	Standard Deviation
(mg/L)	(mg/L)	(mg/L)
8.20	8.19	0.0089

This report was certified only for the instrument we tested. It is allowable to use for study
Intend to use for advertising and referral purpose is prohibited. This report may not be reproduced
other in full, without written approval of the laboratory

-o0o-



Certificate of Calibration

Cert. No.: 24LM193
Page.: 1 of 2

Equipment : DO Meter with Sensor
Manufacturer : Horiba
Model : LAQUA-DO210
Serial No. : HE9M0013
ID No. : UAE.EFM.016/2563(EFM.DO.05/63)
Submitted by : United Analyst and Engineering Consultant Co.,Ltd.
3 Soi Udomsuk 41, Sukhumvit Road,
Bangchak, Phrakhanong,
Bangkok 10260
Location : TPA On Site Calibration Laboratory
Received Order : 24 December 2024
Calibrated Date : 25 December 2024
Ambient Temperature : (26 ± 10) °C
Relative Humidity : (50 ± 30) %
AC Line Voltage : (220 ± 22) V
Calibrated by : Warakorn Lernagatrakul
Approved by :
() Ponpan Palpim
() Suwit Imjai
(✓) Kunchit Promprat
Issue Date : 25 December 2024

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.



Equipment : DO Meter with Sensor
Condition As-Received : Used Item
Reference : 2412-0604WSC-2
Procedure Used :-

Cert. No.: 24LM193
Page.: 2 of 2

Calibration were conducted using in-house calibration procedure CP-OT01 according to comparison with Industrial Platinum Resistance Thermometer (IPRT) into Temperature Bath.
The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

Instrument	Serial No.	Cert. No.	Traceable	Due Date
1) Digital Thermometer	2188080	2411022	TPA	17 Sep 2025

2. This certificate is valid only to the item calibrated on date and place of calibration.
3. This certification is traceable to the International System of Unit.

Remark : TPA : Technology Promotion Association (Thailand - Japan)

Result of Calibration : (*) Without Adjustment
Function : Temperature measurement.

This instrument was connected with temperature sensor, S/N.: 9K9G0097

Calibration Point (°C)	Immersion Depth (mm)	Standard Temperature (°C)	UUC* Reading (°C)	Error (°C)	Uncertainty (± °C)	Coverage Factor k
15.0	80	15.003	15.0	-0.003	0.16	2.00
30.0	80	30.002	29.9	-0.102	0.16	2.00
45.0	80	45.004	44.8	-0.204	0.16	2.00

UUC* : Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-



Cert.No.: 24TW57
Page.: 1 of 2

Certificate of Testing

Equipment : DO Meter
Manufacturer : Horiba
Model : LAQUA-DO210
Serial No. : HE2L0016
ID No. : UAE.EFM.016/2566(EFM.DO.01/66)
Received Date : 12 March 2024
Test Date : 13 March 2024
Reference : 2403-0385WSC-4
Submitted by : United Analyst and Engineering Consultant Co.,Ltd.
3 Soi Udomsuk 41, Sukhumvit Road, Bangchak,
Phrakhanong, Bangkok 10260
Laboratory Condition :
Temperature (25 ± 5) °C
Humidity (50 ± 20) %
Test Procedure : In - house method : CP-CH9
by Comparison Technique with Azide Modification Method
Tested by : Walalak Sirthean
Approved by :
() Pornthippa Tameyakul
() Unnopphol Harachai
(✓) Sathip Meangmai
Issue Date : 15 March 2024



Cert.No.: 24TW57
Page.: 2 of 2

Condition of this result of calibration

1. Reference Standard Instruments :
This certification is traceable to the International System of Unit through the reference standards laboratory of Industrial Calibration Center, Technology Promotion Association (Thailand-Japan).

Instruments	Serial No.	ID No.	Certificate No.	Due Date
1. Burette	-	130BU10	23CG1172	22 Mar 2025
2. Balance	14233821	110RC001	23MM405	16 July 2024

2. Standard Material :-

Material	Manufacturer	Lot.No.	Assay
Sodium Thiosulfate pentahydrate	Merck	AM1763316	100.2%

Result : Dissolved Oxygen Meter Adjustment With Air 100 %
Dissolved Oxygen Probe No.: 9K2J0004

Titration Method (Azide Modification Method)	DO Meter Reading	Standard Deviation
(mg/L)	(mg/L)	(mg/L)
8.18	8.18	0.0084

This report was certified only for the instrument we tested. It is allowable to use for study
Intend to use for advertising and referral purpose is prohibited. This report may not be reproduced
other in full, without written approval of the laboratory

-o0o-



Cert. No.: 24LM42
Page.: 1 of 2

Certificate of Calibration

Equipment : DO Meter With Sensor
Manufacturer : Horiba
Model : LAQUA-DO210
Serial No. : HE2L0016
ID No. : UAE.EFM.016/2566(EFM.DO.01/66)
Submitted by : United Analyst and Engineering Consultant Co.,Ltd.
3 Soi Udomsuk 41, Sukhumvit Road,
Bangchak, Phrakhanong,
Bangkok 10260
Location : TPA Chemistry Calibration Laboratory
Received Order : 12 March 2024
Calibrated Date : 14 March 2024
Ambient Temperature : (26 ± 10) °C
Relative Humidity : (50 ± 30) %
AC Line Voltage : (220 ± 22) V
Calibrated by : Preecha Hlaib
Approved by :
() Pornthippa Tameyakul
() Unnopphol Harachai
(✓) Suwit Imjai
Issue Date : 29 March 2024

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services



Equipment : DO Meter With Sensor
Condition As-Received : Used Item
Reference : 2403-0385WSC-3
Procedure Used :-

Cert. No.: 24LM42
Page.: 2 of 2

Calibration were conducted using in-house calibration procedure CP-OT01 according to comparison with Industrial Platinum Resistance Thermometer (IPRT) into Temperature Bath.
The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

Instrument	Serial No.	Cert. No.	Traceable	Due Date
1) Digital Thermometer	A52847	23/1222	TPA	10 Oct 2024

2. This certificate is valid only to the item calibrated on date and place of calibration.
3. This certificate is traceable to the International System of Unit.

Remark : TPA : Technology Promotion Association (Thailand - Japan)

Result of Calibration :- (*) Without Adjustment

Function : Temperature measurement.

This instrument was connected with temperature sensor, S/N : 9K2J0004

Calibration Point (°C)	Immersion Depth (mm)	Standard Temperature (°C)	UUC* Reading (°C)	Error (°C)	Uncertainty (± °C)	Coverage Factor k
25.0	100	25.003	25.0	-0.003	0.16	2.00
30.0	100	30.003	30.0	-0.003	0.16	2.00
35.0	100	35.003	34.9	-0.103	0.16	2.00

UUC* : Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-



Certificate of Testing

Cert.No.: 25TW36
Page.: 1 of 2

Equipment : DO Meter
Manufacturer : Horiba
Model : LAQUA-DO210
Serial No. : HE2L0040
ID No. : UAE.EFM.017/2566(EFM.DO.02/66)
Received Date : 25 February 2025
Test Date : 26 February 2025
Reference : 2502-0786WSC-3
Submitted by : United Analyst and Engineering Consultant Co.,Ltd.
3 Soi Udomsuk 41, Sukhumvit Road, Bangchak,
Phrakhanong, Bangkok 10260
Laboratory Condition : Temperature (25 ± 5) °C
Humidity (50 ± 20) %
Test Procedure : In - house method : CP-CH9
by Comparison Technique with Azide Modification Method
Tested by : Walalak Sirithean
Approved by :
() Chakrit Waewwanjua
() Ponpan Paipim
(✓) Saithip Meangmai
Issue Date : 27 February 2025



Cert.No.: 25TW36
Page.: 2 of 2

Condition of this result of calibration

1. Reference Standard Instruments :

This certification is traceable to the International System of Unit through the reference standards
Laboratory of Industrial Calibration Center, Technology Promotion Association (Thailand-Japan).

Instruments	Serial No.	ID No.	Certificate No.	Due Date
1. Burette	-	130BU10	23CG1172	22 Mar 2025
2. Balance	14233821	110RC001	24MM131	04 July 2025

2. Standard Material :-

Material	Manufacturer	Lot.No.	Assay
Sodium Thiosulfate 5-Hydrate AR	KEMAUS	2203162447	99.6%

Result : Dissolved Oxygen Meter Adjustment With Air 100 %
Dissolved Oxygen Probe No.: 9K2L0010

Titration Method (Azide Modification Method) (mg/L)	DO Meter Reading (mg/L)	Standard Deviation (mg/L)
8.20	8.20	0.0084

This report was certified only for the instrument we tested.It is allowable to use for study
Intend to use for advertising and referral purpose is prohibited.This report may not be reproduced
other in full, without written approval of the laboratory

-o0o-



Certificate of Calibration

Cert. No.: 25LM28
Page.: 1 of 2

Equipment : DO Meter with Sensor
Manufacturer : Horiba
Model : LAQUA-DO210
Serial No. : HE2L0040
ID No. : UAE.EFM.017/2566(EFM.DO.02/66)
Submitted by : United Analyst and Engineering Consultant Co.,Ltd.
3 Soi Udomsuk 41, Sukhumvit Road,
Bangchak, Phrakhanong, Bangkok 10260
Location : TPA On Site Calibration Laboratory
Received Order : 25 February 2025
Calibrated Date : 26 February 2025
Ambient Temperature : (26 ± 10) °C
Relative Humidity : (50 ± 30) %
AC Line Voltage : (220 ± 22) V
Calibrated by : Warakorn Lernagatrakul
Approved by : 
() Chakrit Waewwanjua
() Suwit Imjai
(✓) Kunchit Promprat
Issue Date : 28 February 2025

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.



Equipment : DO Meter with Sensor
Condition As-Received : Used Item
Reference : 2502-0786WSC-4
Procedure Used :-

Cert. No.: 25LM28
Page.: 2 of 2

Calibration were conducted using in-house calibration procedure CP-OT01 according to comparison with Industrial Platinum Resistance Thermometer (IPRT) into Temperature Bath.
The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

- | Instrument | Serial No. | Cert. No. | Traceable | Due Date |
|------------------------|------------|-----------|-----------|-------------|
| 1) Digital Thermometer | 2188080 | 2411022 | TPA | 17 Sep 2025 |
2. This certificate is valid only to the item calibrated on date and place of calibration.
3. This certification is traceable to the International System of Unit.

Remark : TPA : Technology Promotion Association (Thailand - Japan)

Result of Calibration :- (*) Without Adjustment

Function : Temperature measurement.

This instrument was connected with temperature sensor, S/N: 9K2L0010

Calibration Point (°C)	Immersion Depth (mm)	Standard Temperature (°C)	UUC* Reading (°C)	Error (°C)	Uncertainty (± °C)	Coverage Factor k
15.0	80	15.004	15.0	-0.004	0.16	2.00
30.0	80	30.004	30.0	-0.004	0.16	2.00
45.0	80	45.003	45.1	0.097	0.16	2.00

UUC* : Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-00-



Certificate of Testing

Cert.No.: 25TW25
Page.: 1 of 2

Equipment : DO Meter
Manufacturer : Horiba
Model : LAQUA-DO210
Serial No. : HE1L0034
ID No. : UAE.EFM.018/2565(EFM.DO.02/65)
Received Date : 04 February 2025
Test Date : 05 February 2025
Reference : 2502-0108WSC-4
Submitted by : United Analyst and Engineering Consultant Co.,Ltd.
3 Soi Udomsuk 41, Sukhumvit Road, Bangchak,
Phrakhanong, Bangkok 10260
Laboratory Condition : Temperature (25 ± 5) °C
Humidity (50 ± 20) %
Test Procedure : In - house method : CP-CH9
by Comparison Technique with Azide Modification Method
Tested by : Walalak Sirithean
Approved by : 
() Chakrit Waewwanjua
() Ponpan Paipim
(✓) Saithip Meangmai
Issue Date : 5 February 2025



Cert.No.: 25TW25
Page.: 2 of 2

Condition of this result of calibration

1. Reference Standard Instruments :

This certification is traceable to the International System of Unit through the reference standards
laboratory of Industrial Calibration Center, Technology Promotion Association (Thailand-Japan).

- | Instruments | Serial No. | ID No. | Certificate No. | Due Date |
|-------------|------------|----------|-----------------|--------------|
| 1. Burette | - | 130BU10 | 23CG1172 | 22 Mar 2025 |
| 2. Balance | 14233821 | 110RC001 | 24MM131 | 04 July 2025 |

2. Standard Material :-

Material	Manufacturer	Lot.No.	Assay
Sodium Thiosulfate 5-Hydrate AR	KEMAUS	2203162447	99.6%

Result : Dissolved Oxygen Meter Adjustment With Air 100 %
Dissolved Oxygen Probe No.: 9K1K0075

Titration Method (Azide Modification Method) (mg/L)	DO Meter Reading (mg/L)	Standard Deviation (mg/L)
8.20	8.20	0.0084

This report was certified only for the instrument we tested. It is allowable to use for study
Intend to use for advertising and referral purpose is prohibited. This report may not be reproduced
other in full, without written approval of the laboratory

-00-



Certificate of Calibration

Cert. No.: 25LM18
Page.: 1 of 2

Equipment : DO Meter with Sensor
Manufacturer : Horiba
Model : LAQUA-DO210
Serial No. : HE1L0034
ID No. : UAE.EFM.018/2565(EFM.DO.02/65)
Submitted by : United Analyst and Engineering Consultant Co.,Ltd.
3 Soi Udomsuk 41, Sukhumvit Road,
Bangchak, Phrakhanong,
Bangkok 10260
Location : TPA On Site Calibration Laboratory
Received Order : 04 February 2025
Calibrated Date : 05 February 2025
Ambient Temperature : (26 ± 10) °C
Relative Humidity : (50 ± 30) %
AC Line Voltage : (220 ± 22) V
Calibrated by : Warakorn Lernagtrakul
Approved by :
() Chakrit Waewwanjua
() Suwit Imjai
(✓) Kunchit Promprat
Issue Date : 07 February 2025

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.



Equipment : DO Meter with Sensor
Condition As-Received : Used Item
Reference : 2502-0108WSC-3
Procedure Used :-

Cert. No.: 25LM18
Page.: 2 of 2

Calibration were conducted using in-house calibration procedure CP-OT01 according to comparison with Industrial Platinum Resistance Thermometer (IPRT) into Temperature Bath.
The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

- | Instrument | Serial No. | Cert. No. | Traceable | Due Date |
|------------------------|------------|-----------|-----------|-------------|
| 1) Digital Thermometer | A52847 | 2411189 | TPA | 25 Oct 2025 |
2. This certificate is valid only to the item calibrated on date and place of calibration.
3. This certification is traceable to the International System of Unit.

Remark : TPA : Technology Promotion Association (Thailand - Japan)

Result of Calibration :- (*) Without Adjustment

Function : Temperature measurement.

This instrument was connected with temperature sensor, S/N.: 9K1K0075

Calibration Point (°C)	Immersion Depth (mm)	Standard Temperature (°C)	UUC* Reading (°C)	Error (°C)	Uncertainty (± °C)	Coverage Factor k
15.0	80	15.003	15.0	-0.003	0.16	2.00
30.0	80	30.005	30.0	-0.005	0.16	2.00
45.0	80	45.002	45.0	-0.002	0.16	2.00

UUC* : Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-



Certificate of Testing

Cert.No.: 25TW27
Page.: 1 of 2

Equipment : DO Meter
Manufacturer : Horiba
Model : LAQUA-DO210
Serial No. : HE0H0008
ID No. : UAE.EFM.086/2564(EFM.DO.05/64)
Received Date : 07 February 2025
Test Date : 10 February 2025
Reference : 2502-0256WSC-1
Submitted by : United Analyst and Engineering Consultant Co.,Ltd.
3 Soi Udomsuk 41, Sukhumvit Road, Bangchak,
Phrakhanong, Bangkok 10260
Laboratory Condition : Temperature (25 ± 5) °C
Humidity (50 ± 20) %
Test Procedure : In - house method : CP-CH9
by Comparison Technique with Azide Modification Method
Tested by : Walalak Sirithean
Approved by :
(✓) Chakrit Waewwanjua
() Ponpan Paipim
() Saithip Meangmai
Issue Date : 11 February 2025



Cert.No.: 25TW27
Page.: 2 of 2

Condition of this result of calibration

1. Reference Standard Instruments :

This certification is traceable to the International System of Unit through the reference standards
Laboratory of Industrial Calibration Center, Technology Promotion Association (Thailand-Japan).

Instruments	Serial No.	ID No.	Certificate No.	Due Date
1. Burette	-	130BU10	23CG1172	22 Mar 2025
2. Balance	14233821	110RC001	24MM131	04 July 2025

2. Standard Material :-

Material	Manufacturer	Lot.No.	Assay
Sodium Thiosulfate 5-Hydrate AR	KEMAUS	2203162447	99.6%

Result : Dissolved Oxygen Meter Adjustment With Air 100 %
Dissolved Oxygen Probe No.: 9K0L0009

Titration Method (Azide Modification Method) (mg/L)	DO Meter Reading (mg/L)	Standard Deviation (mg/L)
8.22	8.22	0.0055

This report was certified only for the instrument we tested.It is allowable to use for study
Intend to use for advertising and referral purpose is prohibited.This report may not be reproduced
other in full, without written approval of the laboratory

-o0o-



Certificate of Calibration

Cert. No.: 25LM21
Page.: 1 of 2

Equipment : DO Meter with Sensor
Manufacturer : Horiba
Model : LAQUA-DO210
Serial No. : HE0H0008
ID No. : UAE.EFM.086/2564(EFM.DO.05/64)
Submitted by : United Analyst and Engineering Consultant Co.,Ltd.
3 Soi Udomsuk 41, Sukhumvit Road,
Bangchak, Phrakhanong,
Bangkok 10260
Location : TPA On Site Calibration Laboratory
Received Order : 07 February 2025
Calibrated Date : 10 February 2025
Ambient Temperature : (26 ± 10) °C
Relative Humidity : (50 ± 30) %
AC Line Voltage : (220 ± 22) V

Calibrated by : Warakorn Lernagtrakul

Approved by :

- () Chakrit Waewwanjua
(✓) Suwit Imjai
() Kunchit Promprat

Issue Date : 10 February 2025

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3: Equipment Calibration and Testing Services.



Equipment : DO Meter with Sensor
Condition As-Received : Used Item
Reference : 2502-0256WSC-2
Procedure Used :-

Cert. No.: 25LM21
Page.: 2 of 2

Calibration were conducted using in-house calibration procedure CP-OT01 according to comparison with Industrial Platinum Resistance Thermometer (IPRT) into Temperature Bath.
The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

Instrument	Serial No.	Cert. No.	Traceable	Due Date
1) Digital Thermometer	2188080	241022	TPA	17 Sep 2025

2. This certificate is valid only to the item calibrated on date and place of calibration.
3. This certification is traceable to the International System of Unit.

Remark : TPA : Technology Promotion Association (Thailand - Japan)

Result of Calibration :- (*) Without Adjustment

Function : Temperature measurement.

This instrument was connected with temperature sensor, S/N.: 9K0L0009

Calibration Point (°C)	Immersion Depth (mm)	Standard Temperature (°C)	UUC* Reading (°C)	Error (°C)	Uncertainty (± °C)	Coverage Factor k
15.0	80	15.002	15.0	-0.002	0.16	2.00
30.0	80	30.002	30.0	-0.002	0.16	2.00
45.0	80	45.003	45.0	-0.003	0.16	2.00

UUC* : Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-



Certificate of Testing

Cert.No.: 25TW29
Page.: 1 of 2

Equipment : DO Meter
Manufacturer : YSI
Model : 5100
Serial No. : 11B 101863
ID No. : UAE.WAO.004/2554
Received Date : 14 February 2025
Test Date : 17 February 2025
Reference : 2502-0473DSC-1
Submitted by : United Analyst and Engineering Consultant Co.,Ltd.
3 Soi Udomsuk 41, Sukhumvit Road, Bangchak,
Phrakhanong, Bangkok 10260
Laboratory Condition : Temperature (25 ± 5) °C
Humidity (50 ± 20) %
Test Procedure : In - house method : CP-CH9
by Comparison Technique with Azide Modification Method

Tested by : Walalak Sirithean

Approved by :

- () Chakrit Waewwanjua
() Ponpan Paipim
(✓) Saitthip Meangmai

Issue Date : 18 February 2025



Cert.No.: 25TW29
Page.: 2 of 2

Condition of this result of calibration

1. Reference Standard Instruments :

This certification is traceable to the International System of Unit through the reference standards laboratory of Industrial Calibration Center, Technology Promotion Association (Thailand-Japan).

Instruments	Serial No.	ID No.	Certificate No.	Due Date
1. Burette	-	130BU10	23CG1172	22 Mar 2025
2. Balance	14233821	110RC001	24MM131	04 July 2025

2. Standard Material :-

Material	Manufacturer	Lot.No.	Assay
Sodium Thiosulfate 5-Hydrate AR	KEMAUS	2203162447	99.6%

Result : Dissolved Oxygen Meter Adjustment With Air 100 %
Dissolved Oxygen Probe No.: 24F100202

Titration Method (Azide Modification Method) (mg/L)	DO Meter Reading (mg/L)	Standard Deviation (mg/L)
8.22	8.22	0.0055

This report was certified only for the instrument we tested. It is allowable to use for study
Intend to use for advertising and referral purpose is prohibited. This report may not be reproduced
other in full, without written approval of the laboratory

-o0o-



Certificate of Testing

Cert.No.: 24TW179
Page.: 1 of 2

Equipment :	DO Meter
Manufacturer :	YSL
Model :	Pro 20i
Serial No. :	18F103884
ID No. :	UAE,EFM,199/2561 (ENV.DO, 03/61)
Received Date :	27 August 2024
Test Date :	28 August 2024
Reference :	2408-0883WSC-1
Submitted by :	United Analyst and Engineering Consultant Co.,Ltd. 3 Soi Udumsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Laboratory Condition :	Temperature (25 ± 5) °C Humidity (50 ± 20) %
Test Procedure :	In - house method : CP-CH9 by Comparison Technique with Azide Modification Method
Tested by :	Walalak Sirithean 
Approved by :	<hr/> Approved Signatory

() Unnophol Harachai
() Ponpan Paipim
(✓) Saithip Meangmai

ใบกำกับผลการสอบเทียบ (Verification of Certificate)									
Certificate No.: ZSV129					Equipment : Do Meter				
Brand : VSI					Model : 5100				
Serial No.: 118 101863					ID No.: UAE.WAQ.006/Z554				
Calibration results									
Titration Method	Standard Deviation (mg/L)	Do meter Reading (mg/L)	Error% (mg/L)	Correction% (mg/L)	Error Total Error (mg/L)	Judgement	(Total Error < Judgement)		
8.32	0.0055	8.32	0.0000	0.0000	0.0	0.02	pass		
ผู้สอบเทียบ: สมชาย หงษ์นิมิต									
วันที่: 28/02/2023									
3.92 23.0.14.14									
ขอสงวนสิทธิ์ใน:									

WILEY-INTERSCIENCE, JOHN WILEY & SONS, INC.

เอกสารไม่ควบคุม



Cert.No.: 24TW179
Page.: 2 of 2

Condition of this result of calibration

1. Reference Standard Instruments :
This certification is traceable to the International System of Unit through the reference standards laboratory of Industrial Calibration Center, Technology Promotion Association (Thailand-Japan).

<u>Instruments</u>	<u>Serial No.</u>	<u>ID No.</u>	<u>Certificate No.</u>	<u>Due Date</u>
1. Burette	-	130BU10	23CG1172	22 Mar 2025
2. Balance	N03679	140RC001	23MM537	14 Sep 2024

- ## 2. Standard Material :-

<u>Material</u>	<u>Manufacturer</u>	<u>Lot.No.</u>	<u>Assay</u>
Sodium Thiosulfate 5-Hydrate AR	KEMAUS	2203162447	99.6%

Result : Dissolved Oxygen Meter Adjustment With Air 100 %
Dissolved Oxygen Probe No.: 18F100252

Titration Method (Azide Modification Method) (mg/L)	DO Meter Reading (mg/L)	Standard Deviation (mg/L)
8.20	8.20	0.0055

This report was certified only for the instrument we tested. It is allowable to use for study
Intend to use for advertising and referral purpose is prohibited. This report may not be reproduced
other in full, without written approval of the laboratory

-ooo-



Certificate of Calibration

Cert. No.: 24LM135
Page.: 1 of 2

Equipment : DO Meter with Sensor

Manufacturer : YSI

Model : Pro 20i

Serial No. : 18F103884

ID No. : UAE,EFM,199/2561(ENV.DO,03/61)

Submitted by : United Analyst and Engineering Consultant Co.,Ltd.
3 Soi Udomsuk 41, Sukhumvit Road,
Bangchak, Phrakhanong,
Bangkok 10260

Location : TPA On Site Calibration Laboratory

Received Order : 27 August 2024


Calibrated Date : 28 August 2024

Ambient Temperature : (26 ± 10) °C

Relative Humidity : (50 ± 30) %

AC Line Voltage : (220 ± 22) V

Calibrated by : Warakorn Lernagatrakul


Approved Signatory

() Ponpan Paipim
() Suwit Injai
(✓) Kunchit Promprat

Issue Date : 02 September 2024

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.



Equipment : DO Meter with Sensor
Condition As-Received : Used Item
Reference : 2408-0883WSC-2
Cert. No.: 24LM135
Page.: 2 of 2

Procedure Used :-
Calibration were conducted using in-house calibration procedure CP-OT01 according to comparison with Industrial Platinum Resistance Thermometer (IPRT) into Temperature Bath.

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

Instrument	Serial No.	Cert. No.	Traceable	Due Date
1) Digital Thermometer	2188080	2311216	TPA	11 Oct 2024

2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certification is traceable to the International System of Unit.

Remark : TPA : Technology Promotion Association (Thailand - Japan)

Result of Calibration :- (*) Without Adjustment

Function : Temperature measurement.

This instrument was connected with temperature sensor, S/N.: 18F100252

Calibration Point (°C)	Immersion Depth (mm)	Standard Temperature (°C)	UUC* Reading (°C)	Error (°C)	Uncertainty (± °C)	Coverage Factor k
25.0	80	25.002	24.9	-0.102	0.16	2.00
30.0	80	30.002	29.9	-0.102	0.16	2.00
35.0	80	35.003	34.9	-0.103	0.16	2.00

UUC* : Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3 : EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000 FAX. 0-2719-9484

Cert.No.: 24TW39
Page.: 1 of 2

Certificate of Testing

Equipment : DO Meter
Manufacturer : YSI
Model : 5100
Serial No. : 11B 101863
ID No. : UAE.WAO.004/2554
Received Date : 20 February 2024
Test Date : 21 February 2024
Reference : 2402-0629DSC-1
Submitted by : United Analyst and Engineering Consultant Co.,Ltd.
3 Soi Udumruk 41, Sukhumvit Road, Bangchak,
Phrakhanong, Bangkok 10260
Laboratory Condition : Temperature (25 ± 5) °C
Humidity (50 ± 20) %
Test Procedure : In - house method : CP-CH9
by Comparison Technique with Azide Modification Method

Tested by : Walalak Sirthean

Approved by :
Approved Signatory

() Pornthippa Tameyakul
() Unnophol Harachai
(✓) Saithip Meangmai

Issue Date : 22 February 2024

เอกสารไม่ควบคุม



Cert.No.: 24TW39
Page.: 2 of 2

Condition of this result of calibration

1. Reference Standard Instruments :
This certification is traceable to the International System of Unit through the reference standards laboratory of Industrial Calibration Center, Technology Promotion Association (Thailand-Japan).

Instruments	Serial No.	ID No.	Certificate No.	Due Date
1. Burette	-	130BU10	23CG1172	22 Mar 2025
2. Balance	14233821	110RC001	23MM405	16 July 2024

2. Standard Material :-

Material	Manufacturer	Lot.No.	Assay
Sodium Thiosulfate pentahydrate	Merck	AM1763316	100.2%

Result : Dissolved Oxygen Meter Adjustment With Air 100 %
Dissolved Oxygen Probe No.: 22B100125

Titration Method (Azide Modification Method) (mg/L)	DO Meter Reading (mg/L)	Standard Deviation (mg/L)
8.20	8.19	0.0055

This report was certified only for the instrument we tested. It is allowable to use for study
Intend to use for advertising and referral purpose is prohibited. This report may not be reproduced
other in full, without written approval of the laboratory

-o0o-

เอกสารไม่ควบคุม

FOSS

Customer Service Report

Date:	Jan 27, 2025	Report No.:	13320
Job No.:	11626	Customer:	UAE
Instrument:	DT7520	Address:	Bangkok
		Serial:	91794469
Start	Travel To Customer (Hrs)	Labour (Hrs)	Travel From Customer (Hrs)
Finish	-	13.00 2	-

Application	Special	Standard
Distributor	Courtesy Visit	Installation
Digital Service	PMA Onboarding	Quote
Internal	Warranty	Repair
Investigate	Sales Support	Remote

PMA Type	Smartcare	Smartcare Pro	Fosscore
	Smartcare Advance	Fosscore Pro	N/A

Details of Work / Test
- PM -
- Visual Check -
- No damage -
- No corrosion -
- Function Check -
- Set Temp / Time
- Set Contrast
- Change unit °C / °F
- Re / Reentry 42.0 °C → 42.0 °C
* Wash Auto 114 (LS)

Instrument Ready for Use OK X Not OK*

Part No.	Batch	Description	Qty
60076930		FOSS PM kit, Digital T7520 per 12 months	1

I confirm this report is accurate and complete	
Signed FOSS	Signed Customer
Name	Name

Email: Customer Contact: เอกสารไม่ควบคุม

*Remark:

Agilent CrossLab Start Up Services Agilent 7890 Gas Chromatograph Preventive Maintenance Checklist

Agilent Preventive Maintenance provides factory recommended service for your analytical instruments to assure reliable operation and the accuracy of your results.

Delivered by highly trained and certified service engineers using genuine Agilent parts and supplies, Agilent Preventive Maintenance provides everything you need to reduce unplanned downtime and keep your systems operating at their peak. This checklist will be completed at the end of the service and provided to you as a record of the preventive maintenance activities.

Introduction

Customer Information

- Customers should provide all necessary operating supplies upon request of the engineer.
- A customer representative should be available to the engineer while performing the preventive maintenance procedures.
- Any parts, not included in the Parts Lists section of this document, are not part of the recommended Preventive Maintenance service, nor are they included in the price of this service.
- If a system requires the use of extra or special procedures and/or parts for the maintenance service, then these must be ordered separately and charged as a repair, which may incur additional costs.

Important Customer Web Links

- For more information about **Agilent Technologies services**, please visit our website using the following URL: <http://www.agilent.com/en-us/products/crosslab-instrument-services/service-repair>
- The **Agilent Community** is an excellent place to get answers, collaborate with others about applications and Agilent products, and find in-depth documents and videos relevant to Agilent technologies. Visit <https://community.agilent.com/welcome>.
- To access **Agilent University**, visit <http://www.agilent.com/crosslab/university/> to learn about training options, which include online, classroom and onsite delivery. A training specialist can work directly with you to help determine your best options.
- A useful **Agilent Resource Center** web page is available, which includes short videos on maintenance, quick lists of consumables for new instruments, and other valuable information. Check out the Resource Page here: <https://www.agilent.com/en-us/agilentresources>.
- Need technical support, FAQs, supplies? – visit our **Support Home page** <http://www.agilent.com/search/support>.
- Videos** about specific preparation requirements for your instrument can be found by searching the **Agilent YouTube** channel at <https://www.youtube.com/user/agilent>.
- 7890B Manuals** are also available on Agilent.com:
 - Safety**
https://www.agilent.com/cs/library/usermanuals/public/7890B_Safety.pdf
 - Installation and First Startup**
https://www.agilent.com/cs/library/usermanuals/Public/7890B_Installation.pdf
 - Operation Manual**
https://www.agilent.com/cs/library/usermanuals/Public/7890B_Operation.pdf
 - Maintaining Your GC**
https://www.agilent.com/cs/library/usermanuals/public/G3430-90052%207890B_Maintaining%20Guide.pdf

Revision: 2.00, Issued: December 30, 2020
Agile Document Number: D0007063
DE number: 44166.759722222
© Agilent Technologies, Inc. 2020

Page 2 of 9

เอกสารไม่ควบคุม

เอกสารไม่ควบคุม

Service Engineer's Responsibilities

- Contact the customer and ensure that all necessary supplies are available before the preventive maintenance visit.
- Only select those pages that relate to the system or module being serviced.
- Complete empty fields with the relevant information.
- Complete the relevant checkboxes in the checklist using either a "X" or tick mark "✓".
- Check "Section not applicable" check boxes to indicate services/tasks not delivered, as appropriate.
- Complete the Preventive Maintenance service in the order of the tasks listed.
- Complete the Service Review section together with the customer.
- Complete the fields for page numbers at the foot of each selected page.
- Complete the total number of pages field in the Service Completion section.
- Ask the customer to sign the Service Completion section including the customer's and your signature.**

Additional Instruction Notes

- Check for any active service notes for this unit. If there are any applicable "Safety" or "Modification Recommended" Service notes, plan to implement the changes on this unit before doing any qualification service.
- Do not implement firmware updates, unless you get approval from the customer and are sure that they are compatible with the instrument control software.

Revision: 2.00, Issued: December 30, 2020
Agile Document Number: D0007063
DE number: 44166.759722222
© Agilent Technologies, Inc. 2020

Page 3 of 9

เอกสารไม่ควบคุม

System Information

- ☒ Check this box if an instrument configuration report is attached instead of completing the table below.

Instrument System Name and ID	CN11021007
Instrument System Site and Location	Instrument Room

List System Component Product Numbers	List the Serial Numbers of each Component
1. G3440A	CN11021007
2.	
3.	
4.	
5.	
6.	
7.	
8.	
9.	
10.	

Preparation

- ☒ Discuss any specific issues with the customer before starting.
- ☒ Review the instrument logbook for recorded problems and comments.
- ☒ Save instrument control settings before starting the procedure.
- ☒ Perform a general inspection of the system for cleanliness.
- ☒ Check for proper installation of parts, assemblies, sensors etc.
- ☒ Check system for required installation of components, settings as defined by current Service Notes.
- ☒ Check for required firmware updates and verify with customers if they would like them installed.
- ☒ Before starting the following procedures, record the Detector Signal Output(s) in the results table. If the GC is turned OFF or in a service mode, comparing the detector outputs before and after the service is not possible.

Revision: 2.00, Issued: December 30, 2020
Agile Document Number: D0007063
DE number: 44166.759722222
© Agilent Technologies, Inc. 2020

Page 4 of 9

เอกสารไม่ควบคุม

Preventive Maintenance Procedure

Clean and inspect GC

- ☒ Unplug power cord from the power source.
- ☒ Open GC covers and vacuum/remove any dust/debris. Pay particular attention to cooling fans.
- ☒ Inspect internal connectors for proper contact and placement.
- ☒ Reconnect Power to the GC. Power the GC on and verify the power on self-test passed.
- ☒ Verify oven motor spins freely and turns on with the oven door closed; off when the door is opened.
- ☒ Verify operation of all other fans - the inlet and EPC cooling fans.
- ☒ Verify oven intake/outlet flap assembly is operating smoothly while heating and cooling the oven

Inlet and detector consumable replacement

- ☒ For the inlets installed, perform inlet maintenance as defined in the 7890 manual - "Maintaining Your GC" - for the inlet(s) installed.
- ☒ Replace the split vent trap cartridge filter on units with these inlets: Split/Splitless Capillary (SSL), Multi-Mode Inlet (MMI), Programmed Temperature Vaporizer (PTV), Volatile Interface (VI).
- ☒ If the inlet system is used in Split Mode with viscous samples, inspect and clean the split vent tube on the inlet and flush or replace the tubing between the inlet and the split vent trap.
- ☒ If the GC includes a Flame Ionization Detector (FID), replace the jet. If the ignitor shows any buildup of sample or corrosion, replace the ignitor. Examine the FID collector and castle assemblies for contamination - clean as necessary.

Zero Sensors and Leak test

- ☒ Zero all pressure sensors per the procedure in the 7890 "Advanced User Guide".
- ☒ Perform inlet pressure decay test(s) as defined in the 7890 "Troubleshooting Manual". If the PM is done in preparation for an Operational Qualification, then the pressure decay test defined within that protocol can be used for the PM.
- ☒ Record if test passed or failed in the results table.

Revision: 2.00, Issued: December 30, 2020
Agile Document Number: D0007063
DE number: 44166.759722222
© Agilent Technologies, Inc. 2020

Page 5 of 9



เอกสารไม่ควบคุม

ALS Maintenance

- ☒ **Section NOT applicable**
- ☒ Check all cabling and configuration settings between GC, tray, and injectors.
- ☒ Vacuum or remove any dust, especially around fans.
- ☒ Check operation of all fans.
- ☒ Check syringe for smooth plunger operation.
- ☒ Check for smooth operation of the needle support - clean if necessary

Restore Instrument

- ☒ Restore the normal operating conditions or customer method using the Browser interface or Data System.
- ☒ Purge the system with carrier flow for 15 minutes
- ☒ Bake out the system, then restore the normal operating conditions
- ☒ After equilibration, check and record the post PM detector signal output values. Results should be similar or lower than the detector outputs recorded prior to PM.
- ☒ Perform a chemical checkout. If this is a routine PM, inject the customer's sample using the ALS if applicable. This will act as a final checkout of both the ALS and the GC.

Note: If the PM Service is performed prior to a qualification service, then use the qualification procedure as a guide for final instrument set up and checkout.

Revision: 2.00, Issued: December 30, 2020
Agile Document Number: D0007063
DE number: 44166.759722222
© Agilent Technologies, Inc. 2020

Page 6 of 9



เอกสารไม่ควบคุม

Signature Page

Service Review


- ☒ Attach available reports/printouts of all tests to this documentation.
- ☒ Record the Preventive Maintenance service activity in the customer's records/logbook.
- ☒ Update/reset Instrument maintenance counters as appropriate.
- ☒ Affix the PM sticker to the system or instrument logbook based on the customer's request.
- ☒ Complete the Service Engineer Comments section if there are additional comments.
- ☒ Review with the customer this service, parts replaced, and test results obtained.
- ☒ If the instrument firmware was updated, record the details of the change in the Service Engineer's Comments box or if necessary, in the customer's IQ records.
- ☐ Supply the customer with a copy of the Smart Alerts flyer.
- ☐ Describe Smart Alerts to the customer.
- ☐ Install Smart Alerts if requested.

7890 GC Test Results Table

Detector Signal Outputs	Before PM Service	After PM Service
Front detector output	NA.	NA.
Back detector output	NA.	22.0
AUX detector output	NA.	NA.
Pressure decay test	Expected test result	Actual test result
Front inlet pressure decay test	Pass	Pass
Back inlet pressure decay test	Pass	NA.

Revision: 2.00, Issued: December 30, 2020
Agile Document Number: D0007063
DE number: 44166.759722222
© Agilent Technologies, Inc. 2020

Page 7 of 9



เอกสารไม่ควบคุม

7890 Parts List Table

The following kits are recommended for capillary and purged packed inlets. If this is a general PM and the customer has a preferred set of consumables, you may use the customer's consumables.

Part description	Part number	Product or model# where used	Quantity consumed
SSL Capillary Inlet PM kit, Splitless	5188-6497	7890A/B	1
SSL Capillary Inlet PM kit, split	5188-6496	7890A/B	
SSL Capillary Ultra Inert Inlet Gold Seal with Washer	5190-6144	7890A/B	
SSL Capillary Ultra Inert Inlet Splitless Liner - Single taper with Glass Wool	5190-2293	7890A/B	
SSL Capillary Ultra Inert Inlet Low Pressure Drop Split Liner - with Glass Wool	5190-2295	7890A/B	
PP Inlet PM kit	5188-6498	7890A/B	
Split vent trap PM kit, single cartridge (for MMI, PTV & VI)	5188-6495	7890A/B	
MMI Cleaning Kit	G3510-60820	7890A/B	
PTV Septumless Head Rebuild Kit	5182-9747	7890A/B	
PTV Septumless Head Teflon Guide	5182-9748	7890A/B	
Ignitor (glow plug) assembly with O-ring	19231-60680	7890A/B	1
FID Collector Rebuild/Cleaning Kit	G1531-67000	7890A/B	
Standard .011-inch FID Jet for capillary FID base	G1531-80560	7890A/B	1
High Temperature .018-inch FID Jet for capillary FID base	G1531-80620	7890A/B	
Standard .018-inch FID Jet for packed column with packed FID base	18710-20119	7890A/B	
Standard .011-inch FID Jet for capillary column with packed/adaptable FID base	19244-80560	7890A/B	
High Temperature .018-inch FID Jet for capillary column with packed/adaptable FID base	19244-80620	7890A/B	
NPD Jet, universal fit, .011-inch ID	G1534-80580	7890A/B	
NPD Jet, universal fit, .011-inch ID Extended tip	G1534-80590	7890A/B	
SSL Capillary Ultra Inert Inlet Gold Seal with Washer	5190-6144	7890A/B	
SSL Capillary Ultra Inert Inlet Splitless Liner - Single taper with Glass Wool	5190-2293	7890A/B	
**FID Collector Replacement Kit, if needed	G1531-67001	7890A/B	

Revision: 2.00, Issued: December 30, 2020
Agile Document Number: D0007063
DE number: 44166.759722222
© Agilent Technologies, Inc. 2020

Page 8 of 9



เอกสารไม่ควบคุม


Service Engineer Comments

If there are any specific points you wish to note as part of performing the service or other items of interest for the customer, please write include them in this box.

Service Completion

Service request number 6006748380 Date service completed 21Feb2024
 Agilent signature Phuwana Yoktragul Customer signature _____
 Total number of pages in this document 9

Revision: 2.00, Issued: December 30, 2020
 Agile Document Number: D0007063
 DE number: 44166.759722222
 © Agilent Technologies, Inc. 2020

Page 9 of 9

เอกสารไม่ควบคุม

Agilent CrossLab Start Up Services

Agilent 7890 Gas Chromatograph

Preventive Maintenance Checklist

Agilent Preventive Maintenance provides factory recommended service for your analytical instruments to assure reliable operation and the accuracy of your results.

Delivered by highly trained and certified service engineers using genuine Agilent parts and supplies, Agilent Preventive Maintenance provides everything you need to reduce unplanned downtime and keep your systems operating at their peak. This checklist will be completed at the end of the service and provided to you as a record of the preventive maintenance activities.



เอกสารไม่ควบคุม

Introduction

Customer Information

- Customers should provide all necessary operating supplies upon request of the engineer.
- A customer representative should be available to the engineer while performing the preventive maintenance procedures.
- Any parts, not included in the Parts Lists section of this document, are not part of the recommended Preventive Maintenance service, nor are they included in the price of this service.
- If a system requires the use of extra or special procedures and/or parts for the maintenance service, then these must be ordered separately and charged as a repair, which may incur additional costs.

Important Customer Web Links

- For more information about **Agilent Technologies services**, please visit our website using the following URL: <http://www.agilent.com/en-us/products/crosslab-instrument-services/service-repair>
- The **Agilent Community** is an excellent place to get answers, collaborate with others about applications and Agilent products, and find in-depth documents and videos relevant to Agilent technologies. Visit <https://community.agilent.com/welcome>.
- To access **Agilent University**, visit <http://www.agilent.com/crosslab/university/> to learn about training options, which include online, classroom and onsite delivery. A training specialist can work directly with you to help determine your best options.
- A useful **Agilent Resource Center** web page is available, which includes short videos on maintenance, quick lists of consumables for new instruments, and other valuable information. Check out the Resource Page here: <https://www.agilent.com/en-us/agilentresources>.
- Need technical support, FAQs, supplies? – visit our **Support Home page** <http://www.agilent.com/search/support>.
- Videos** about specific preparation requirements for your instrument can be found by searching the **Agilent YouTube** channel at <https://www.youtube.com/user/agilent>.
- 7890B Manuals** are also available on Agilent.com:
 - Safety**
https://www.agilent.com/cs/library/usermanuals/public/7890B_Safety.pdf
 - Installation and First Startup**
https://www.agilent.com/cs/library/usermanuals/Public/7890B_Installation.pdf
 - Operation Manual**
https://www.agilent.com/cs/library/usermanuals/Public/7890B_Operation.pdf
 - Maintaining Your GC**
https://www.agilent.com/cs/library/usermanuals/public/G3430-90052%207890B_Maintaining%20Guide.pdf

Revision: 2.01, Issued: September 15, 2021
 Agile Document Number: D0013618
 DE number: 44166.759722222
 © Agilent Technologies, Inc. 2021

Page 1 of 8

เอกสารไม่ควบคุม

Service Engineer's Responsibilities

- Contact the customer and ensure that all necessary supplies are available before the preventive maintenance visit.
- Only select those pages that relate to the system or module being serviced.
- Complete empty fields with the relevant information.
- Complete the relevant checkboxes in the checklist using either a "X" or tick mark "✓".
- Check **"Section not applicable"** check boxes to indicate services/tasks not delivered, as appropriate.
- Complete the Preventive Maintenance service in the order of the tasks listed.
- Complete the Service Review section together with the customer.
- Complete the fields for page numbers at the foot of each selected page
- Complete the total number of pages field in the Service Completion section
- Ask the customer to sign the Service Completion section including the customer's and your signature.**

Additional Instruction Notes

- Check for any active service notes for this unit. If there are any applicable "Safety" or "Modification Recommended" Service notes, plan to implement the changes on this unit before doing any qualification service.
- Do not implement firmware updates, unless you get approval from the customer and are sure that they are compatible with the instrument control software.

Revision: 2.01, Issued: September 15, 2021
 Agile Document Number: D0013618
 DE number: 44166.759722222
 © Agilent Technologies, Inc. 2021

Page 2 of 8

เอกสารไม่ควบคุม

System Information

☑ Check this box if an instrument configuration report is attached instead of completing the table below.

Instrument System Name and ID	UAE_TOX.007
Instrument System Site and Location	Laboratory

List System Component Product Numbers	List the Serial Numbers of each Component
1. G3440A	CN11021007
2. G4513A	CN20030059
3. G4514A	CN20020060
4.	
5.	
6.	
7.	
8.	
9.	
10.	

Preparation

- ☑ Discuss any specific issues with the customer before starting.
- ☑ Review the instrument logbook for recorded problems and comments.
- ☑ Save instrument control settings before starting the procedure.
- ☑ Perform a general inspection of the system for cleanliness.
- ☑ Check for proper installation of parts, assemblies, sensors etc.
- ☑ Check system for required installation of components, settings as defined by current Service Notes.
- ☑ Check for required firmware updates and verify with customers if they would like them installed.
- ☑ Before starting the following procedures, record the Detector Signal Output(s) in the results table. If the GC is turned OFF or in a service mode, comparing the detector outputs before and after the service is not possible.

Revision: 2.01, Issued: September 15, 2021
 Agile Document Number: D0013618
 DE number: 44166.759722222
 © Agilent Technologies, Inc. 2021

Page 3 of 8



เอกสารไม่ควบคุม

Preventive Maintenance Procedure

Clean and inspect GC

- ☑ Unplug power cord from the power source.
- ☑ Open GC covers and vacuum/remove any dust/debris. Pay particular attention to cooling fans.
- ☑ Inspect internal connectors for proper contact and placement.
- ☑ Reconnect Power to the GC. Power the GC on and verify the power on self-test passed.
- ☑ Verify oven motor spins freely and turns on with the oven door closed; off when the door is opened.
- ☑ Verify operation of all other fans - the inlet and EPC cooling fans.
- ☑ Verify oven intake/outlet flap assembly is operating smoothly while heating and cooling the oven

Inlet and detector consumable replacement

- ☑ For the inlets installed, perform inlet maintenance as defined in the 7890 manual - "Maintaining Your GC" - for the inlet(s) installed.
- ☑ Replace the split vent trap cartridge filter on units with these inlets: Split/Splitless Capillary (SSL), Multi-Mode Inlet (MMI), Programmed Temperature Vaporizer (PTV), Volatiles Interface (VI).
- ☑ If the inlet system is used in Split Mode with viscous samples, inspect and clean the split vent tube on the inlet and flush or replace the tubing between the inlet and the split vent trap.
- ☑ If the GC includes a Flame Ionization Detector (FID), replace the jet. If the ignitor shows any buildup of sample or corrosion, replace the ignitor. Examine the FID collector and castle assemblies for contamination - clean as necessary.

Zero Sensors and Leak test

- ☑ Zero all pressure sensors per the procedure in the 7890 "Advanced User Guide".
- ☑ Perform inlet pressure decay test(s) as defined in the 7890 "Troubleshooting Manual". If the PM is done in preparation for an Operational Qualification, then the pressure decay test defined within that protocol can be used for the PM.
- ☑ Record if test passed or failed in the results table.

Revision: 2.01, Issued: September 15, 2021
 Agile Document Number: D0013618
 DE number: 44166.759722222
 © Agilent Technologies, Inc. 2021

Page 4 of 8



เอกสารไม่ควบคุม

ALS Maintenance

- ☐ Section NOT applicable
- ☑ Check all cabling and configuration settings between GC, tray, and injectors.
- ☑ Vacuum or remove any dust, especially around fans.
- ☑ Check operation of all fans.
- ☑ Check syringe for smooth plunger operation.
- ☑ Check for smooth operation of the needle support - clean if necessary

Restore Instrument

- ☑ Restore the normal operating conditions or customer method using the Data System.
- ☑ Purge the system with carrier flow for 15 minutes
- ☑ Bake out the system, then restore the normal operating conditions
- ☑ After equilibration, check and record the post PM detector signal output values. Results should be similar or lower than the detector outputs recorded prior to PM.
- ☑ Perform a chemical checkout. If this is a routine PM, inject the customer's sample using the ALS if applicable. This will act as a final checkout of both the ALS and the GC.

Note: If the PM Service is performed prior to a qualification service, then use the qualification procedure as a guide for final instrument set up and checkout.

Revision: 2.01, Issued: September 15, 2021
 Agile Document Number: D0013618
 DE number: 44166.759722222
 © Agilent Technologies, Inc. 2021

Page 5 of 8



เอกสารไม่ควบคุม

Signature Page

Service Review

- ☑ Attach available reports/printouts of all tests to this documentation.
- ☑ Record the Preventive Maintenance service activity in the customer's records/logbook.
- ☑ Update/reset instrument maintenance counters as appropriate.
- ☑ Affix the PM sticker to the system or instrument logbook based on the customer's request.
- ☑ Complete the Service Engineer Comments section if there are additional comments.
- ☑ Review with the customer this service, parts replaced, and test results obtained.
- ☑ If the instrument firmware was updated, record the details of the change in the Service Engineer's Comments box or if necessary, in the customer's IQ records.
- ☐ Supply the customer with a copy of the Smart Alerts flyer.
- ☐ Describe Smart Alerts to the customer.
- ☐ Install Smart Alerts if requested.

7890 GC Test Results Table

Detector Signal Outputs	Before PM Service	After PM Service
Front detector output	313.5	313.5
Back detector output	24.5	19.3
AUX detector output	n/a	n/a
Pressure decay test	Expected test result	Actual test result
Front inlet pressure decay test	Pass	Pass
Back inlet pressure decay test	Pass	n/a

Revision: 2.01, Issued: September 15, 2021
 Agile Document Number: D0013618
 DE number: 44166.759722222
 © Agilent Technologies, Inc. 2021

Page 6 of 8



เอกสารไม่ควบคุม

7890 Parts List Table

The following kits are recommended for capillary and purged packed inlets. If this is a general PM and the customer has a preferred set of consumables, you may use the customer's consumables.

Part description	Part number	Product or model# where used	Quantity consumed
SSL Capillary Inlet PM kit, Splitless	5188-6497	7890A/B	1
SSL Capillary Inlet PM kit, split	5188-6496	7890A/B	-
SSL Capillary Ultra Inert Inlet Gold Seal with Washer	5190-6144	7890A/B	-
SSL Capillary Ultra Inert Inlet Splitless Liner - Single taper with Glass Wool	5190-2293	7890A/B	-
SSL Capillary Ultra Inert Inlet Low Pressure Drop Split Liner - with Glass Wool	5190-2295	7890A/B	-
PP Inlet PM kit	5188-6498	7890A/B	-
Split vent trap PM kit, single cartridge (for MMI, PTV & VI)	5188-6495	7890A/B	-
MMI Cleaning Kit	G3510-60820	7890A/B	-
PTV Septumless Head Rebuild Kit	5182-9747	7890A/B	-
PTV Septumless Head Teflon Guide	5182-9748	7890A/B	-
Ignitor (glow plug) assembly with O-ring	19231-60680	7890A/B	1
FID Collector Rebuild/Cleaning Kit	G1531-67000	7890A/B	-
Standard .011-inch FID Jet for capillary FID base	G1531-80560	7890A/B	-
High Temperature .018-inch FID Jet for capillary FID base	G1531-80620	7890A/B	-
Standard .018-inch FID Jet for packed column with packed FID base	18710-20119	7890A/B	-
Standard .011-inch FID Jet for capillary column with packed/adaptable FID base	19244-80560	7890A/B	1
High Temperature .018-inch FID Jet for capillary column with packed/adaptable FID base	19244-80620	7890A/B	-
NPD Jet, universal fit, .011-inch ID	G1534-80580	7890A/B	-
NPD Jet, universal fit, .011-inch ID Extended tip	G1534-80590	7890A/B	-
SSL Capillary Ultra Inert Inlet Gold Seal with Washer	5190-6144	7890A/B	-
SSL Capillary Ultra Inert Inlet Splitless Liner - Single taper with Glass Wool	5190-2293	7890A/B	-
**FID Collector Replacement Kit, if needed	G1531-67001	7890A/B	-

Revision: 2.01, Issued: September 15, 2021
Agile Document Number: D0013618
DE number: 44166.759722222
© Agilent Technologies, Inc. 2021

Page 7 of 8



เอกสารไม่ควบคุม

Service Engineer Comments

If there are any specific points you wish to note as part of performing the service or other items of interest for the customer, please write include them in this box.

- The Equipment can operate as normally.

Service Completion

Service request number 6007319635 Date service completed 18 Feb 2025
Agilent signature Adirek R. Customer signature _____
Total number of pages in this document 9

Revision: 2.01, Issued: September 15, 2021
Agile Document Number: D0013618
DE number: 44166.759722222
© Agilent Technologies, Inc. 2021

Page 8 of 8



เอกสารไม่ควบคุม

Agilent CrossLab Start Up Services

Agilent 7890 Gas Chromatograph Preventive Maintenance Checklist

Agilent Preventive Maintenance provides factory recommended service for your analytical instruments to assure reliable operation and the accuracy of your results.

Delivered by highly trained and certified service engineers using genuine Agilent parts and supplies, Agilent Preventive Maintenance provides everything you need to reduce unplanned downtime and keep your systems operating at their peak. This checklist will be completed at the end of the service and provided to you as a record of the preventive maintenance activities.

Introduction

Customer Information

- Customers should provide all necessary operating supplies upon request of the engineer.
- A customer representative should be available to the engineer while performing the preventive maintenance procedures.
- Any parts, not included in the Parts Lists section of this document, are not part of the recommended Preventive Maintenance service, nor are they included in the price of this service.
- If a system requires the use of extra or special procedures and/or parts for the maintenance service, then these must be ordered separately and charged as a repair, which may incur additional costs.

Important Customer Web Links

- For more information about **Agilent Technologies services**, please visit our website using the following URL: <http://www.agilent.com/en-us/products/crosslab-instrument-services/service-repair>
- The **Agilent Community** is an excellent place to get answers, collaborate with others about applications and Agilent products, and find in-depth documents and videos relevant to Agilent technologies. Visit <https://community.agilent.com/welcome>.
- To access **Agilent University**, visit <http://www.agilent.com/crosslab/university/> to learn about training options, which include online, classroom and onsite delivery. A training specialist can work directly with you to help determine your best options.
- A useful **Agilent Resource Center** web page is available, which includes short videos on maintenance, quick lists of consumables for new instruments, and other valuable information. Check out the Resource Page here: <https://www.agilent.com/en-us/agilentresources>.
- Need technical support, FAQs, supplies? – visit our **Support Home page** <http://www.agilent.com/search/support>.
- Videos** about specific preparation requirements for your instrument can be found by searching the **Agilent YouTube** channel at <https://www.youtube.com/user/agilent>.
- 7890B Manuals** are also available on Agilent.com:
 - Safety** https://www.agilent.com/cs/library/usermanuals/public/7890B_Safety.pdf
 - Installation and First Startup** https://www.agilent.com/cs/library/usermanuals/Public/7890B_Installation.pdf
 - Operation Manual** https://www.agilent.com/cs/library/usermanuals/Public/7890B_Operation.pdf
 - Maintaining Your GC** https://www.agilent.com/cs/library/usermanuals/public/G3430-90052%207890B_Maintaining%20Guide.pdf

Revision: 2.01, Issued: September 15, 2021
Agile Document Number: D0013618
DE number: 44166.759722222
© Agilent Technologies, Inc. 2021

Page 1 of 8



เอกสารไม่ควบคุม

เอกสารไม่ควบคุม

Service Engineer's Responsibilities

- Contact the customer and ensure that all necessary supplies are available before the preventive maintenance visit.
- Only select those pages that relate to the system or module being serviced.
- Complete empty fields with the relevant information.
- Complete the relevant checkboxes in the checklist using either a "X" or tick mark "✓".
- Check "Section not applicable" check boxes to indicate services/tasks not delivered, as appropriate.
- Complete the Preventive Maintenance service in the order of the tasks listed.
- Complete the Service Review section together with the customer.
- Complete the fields for page numbers at the foot of each selected page
- Complete the total number of pages field in the Service Completion section
- **Ask the customer to sign the Service Completion section including the customer's and your signature.**

Additional Instruction Notes

- Check for any active service notes for this unit. If there are any applicable "Safety" or "Modification Recommended" Service notes, plan to implement the changes on this unit before doing any qualification service.
- Do not implement firmware updates, unless you get approval from the customer and are sure that they are compatible with the instrument control software.

Revision: 2.01, Issued: September 15, 2021
 Agile Document Number: D0013618
 DE number: 44166 759722222
 © Agilent Technologies, Inc. 2021

Page 2 of 8



เอกสารไม่ควบคุม

System Information

- ☑ Check this box if an instrument configuration report is attached instead of completing the table below.

Instrument System Name and ID	UAE.TOX.021
Instrument System Site and Location	Laboratory

List System Component Product Numbers	List the Serial Numbers of each Component
1. G3440B	CN13113001
2. G4513A	CN22285355
3. G4514A	CN13200169
4.	
5.	
6.	
7.	
8.	
9.	
10.	

Preparation

- ☑ Discuss any specific issues with the customer before starting.
- ☑ Review the instrument logbook for recorded problems and comments.
- ☑ Save instrument control settings before starting the procedure.
- ☑ Perform a general inspection of the system for cleanliness.
- ☑ Check for proper installation of parts, assemblies, sensors etc.
- ☑ Check system for required installation of components, settings as defined by current Service Notes.
- ☑ Check for required firmware updates and verify with customers if they would like them installed.
- ☑ Before starting the following procedures, record the Detector Signal Output(s) in the results table. If the GC is turned OFF or in a service mode, comparing the detector outputs before and after the service is not possible.

Revision: 2.01, Issued: September 15, 2021
 Agile Document Number: D0013618
 DE number: 44166 759722222
 © Agilent Technologies, Inc. 2021

Page 3 of 8



เอกสารไม่ควบคุม

Preventive Maintenance Procedure

Clean and inspect GC

- ☑ Unplug power cord from the power source.
- ☑ Open GC covers and vacuum/remove any dust/debris. Pay particular attention to cooling fans.
- ☑ Inspect internal connectors for proper contact and placement.
- ☑ Reconnect Power to the GC. Power the GC on and verify the power on self-test passed.
- ☑ Verify oven motor spins freely and turns on with the oven door closed; off when the door is opened.
- ☑ Verify operation of all other fans - the inlet and EPC cooling fans.
- ☑ Verify oven intake/outlet flap assembly is operating smoothly while heating and cooling the oven

Inlet and detector consumable replacement

- ☑ For the inlets installed, perform inlet maintenance as defined in the 7890 manual – "Maintaining Your GC" – for the inlet(s) installed.
- ☑ Replace the split vent trap cartridge filter on units with these inlets: Split/Spittless Capillary (SSL), Multi-Mode Inlet (MMI), Programmed Temperature Vaporizer (PTV), Volatiles Interface (VI).
- ☑ If the inlet system is used in Split Mode with viscous samples, inspect and clean the split vent tube on the inlet and flush or replace the tubing between the inlet and the split vent trap.
- ☑ If the GC includes a Flame Ionization Detector (FID), replace the jet. If the ignitor shows any buildup of sample or corrosion, replace the ignitor. Examine the FID collector and castle assemblies for contamination – clean as necessary.

Zero Sensors and Leak test

- ☑ Zero all pressure sensors per the procedure in the 7890 "Advanced User Guide".
- ☑ Perform inlet pressure decay test(s) as defined in the 7890 "Troubleshooting Manual". If the PM is done in preparation for an Operational Qualification, then the pressure decay test defined within that protocol can be used for the PM.
- ☑ Record if test passed or failed in the results table.

Revision: 2.01, Issued: September 15, 2021
 Agile Document Number: D0013618
 DE number: 44166 759722222
 © Agilent Technologies, Inc. 2021

Page 4 of 8



เอกสารไม่ควบคุม

ALS Maintenance

- ☐ Section NOT applicable
- ☑ Check all cabling and configuration settings between GC, tray, and injectors.
- ☑ Vacuum or remove any dust, especially around fans.
- ☑ Check operation of all fans.
- ☑ Check syringe for smooth plunger operation.
- ☑ Check for smooth operation of the needle support – clean if necessary

Restore Instrument

- ☑ Restore the normal operating conditions or customer method using the Data System.
- ☑ Purge the system with carrier flow for 15 minutes
- ☑ Bake out the system, then restore the normal operating conditions
- ☑ After equilibration, check and record the post PM detector signal output values. Results should be similar or lower than the detector outputs recorded prior to PM.
- ☑ Perform a chemical checkout. If this is a routine PM, inject the customer's sample using the ALS if applicable. This will act as a final checkout of both the ALS and the GC.

Note: If the PM Service is performed prior to a qualification service, then use the qualification procedure as a guide for final instrument set up and checkout.

Revision: 2.01, Issued: September 15, 2021
 Agile Document Number: D0013618
 DE number: 44166 759722222
 © Agilent Technologies, Inc. 2021

Page 5 of 8



เอกสารไม่ควบคุม

Signature Page

Service Review

- ☒ Attach available reports/printouts of all tests to this documentation.
- ☒ Record the Preventive Maintenance service activity in the customer's records/logbook.
- ☒ Update/reset instrument maintenance counters as appropriate.
- ☒ Affix the PM sticker to the system or instrument logbook based on the customer's request.
- ☒ Complete the Service Engineer Comments section if there are additional comments.
- ☒ Review with the customer this service, parts replaced, and test results obtained.
- ☐ If the instrument firmware was updated, record the details of the change in the Service Engineer's Comments box or if necessary, in the customer's IQ records.
- ☐ Supply the customer with a copy of the Smart Alerts flyer.
- ☐ Describe Smart Alerts to the customer.
- ☐ Install Smart Alerts if requested.

7890 GC Test Results Table

Detector Signal Outputs	Before PM Service	After PM Service
Front detector output	23.5	23.5
Back detector output	n/a	n/a
AUX detector output	n/a	n/a
Pressure decay test	Expected test result	Actual test result
Front inlet pressure decay test	Pass	Pass
Back inlet pressure decay test	Pass	n/a

Revision: 2.01, Issued: September 15, 2021
 Agile Document Number: D0013618
 DE number: 44166.759722222
 © Agilent Technologies, Inc. 2021

Page 6 of 8



เอกสารไม่ควบคุม

7890 Parts List Table

The following kits are recommended for capillary and purged packed inlets. If this is a general PM and the customer has a preferred set of consumables, you may use the customer's consumables.

Part description	Part number	Product or model# where used	Quantity consumed
SSL Capillary Inlet PM kit, Splitless	5188-6497	7890A/B	1
SSL Capillary Inlet PM kit, split	5188-6496	7890A/B	-
SSL Capillary Ultra Inert Inlet Gold Seal with Washer	5190-6144	7890A/B	-
SSL Capillary Ultra Inert Inlet Splitless Liner - Single taper with Glass Wool	5190-2293	7890A/B	-
SSL Capillary Ultra Inert Inlet Low Pressure Drop Split Liner - with Glass Wool	5190-2295	7890A/B	-
PP Inlet PM kit	5188-6498	7890A/B	-
Split vent trap PM kit, single cartridge (for MMI, PTV & VI)	5188-6495	7890A/B	-
MMI Cleaning Kit	G3510-60820	7890A/B	-
PTV Septumless Head Rebuild Kit	5182-9747	7890A/B	-
PTV Septumless Head Teflon Guide	5182-9748	7890A/B	-
Ignitor (glow plug) assembly with O-ring	19231-60680	7890A/B	-
FID Collector Rebuild/Cleaning Kit	G1531-67000	7890A/B	-
Standard .011-inch FID Jet for capillary FID base	G1531-80560	7890A/B	1
High Temperature .018-inch FID Jet for capillary FID base	G1531-80620	7890A/B	-
Standard .018-inch FID Jet for packed column with packed FID base	18710-20119	7890A/B	-
Standard .011-inch FID Jet for capillary column with packed/adaptable FID base	19244-80560	7890A/B	-
High Temperature .018-inch FID Jet for capillary column with packed/adaptable FID base	19244-80620	7890A/B	-
NPD Jet, universal fit, .011-inch ID	G1534-80580	7890A/B	-
NPD Jet, universal fit, .011-inch ID Extended tip	G1534-80590	7890A/B	-
SSL Capillary Ultra Inert Inlet Gold Seal with Washer	5190-6144	7890A/B	-
SSL Capillary Ultra Inert Inlet Splitless Liner - Single taper with Glass Wool	5190-2293	7890A/B	-
**FID Collector Replacement Kit, if needed	G1531-67001	7890A/B	-

Revision: 2.01, Issued: September 15, 2021
 Agile Document Number: D0013618
 DE number: 44166.759722222
 © Agilent Technologies, Inc. 2021

Page 7 of 8



เอกสารไม่ควบคุม

Service Engineer Comments

If there are any specific points you wish to note as part of performing the service or other items of interest for the customer, please write include them in this box.

- The Equipment can operate as normally.

Service Completion

Service request number 6007521609 Date service completed 1 APR 2025

Agilent signature Adisak R. Customer signature _____

Total number of pages in this document 9

Revision: 2.01, Issued: September 15, 2021
 Agile Document Number: D0013618
 DE number: 44166.759722222
 © Agilent Technologies, Inc. 2021

Page 8 of 8



เอกสารไม่ควบคุม



Hanna Instruments (Thailand) Ltd.
 410/67-68 Soi Ratchadapisek 24, Ratchadapisek Rd., Samsen-ook,
 Huaykwang, Bangkok 10310 Tel: 0-2541-4199 Fax: 0-2541-4198



ANAB
 ACCREDITED
 CALIBRATION LABORATORY
 AC-3861

Certificate No.: HIT-2412-0389
Page: 1 of 2

CERTIFICATE OF CALIBRATION

Equipment :	COD Test Tube Heater		
Meter Model :	HI839800-02	Serial No. :	H0185001
Tube Heater :	25 Vial Capacity	Resolution :	0.1°C
Temperature Range :	(-10 to 160)°C	Temperature of Reaction :	150°C
Manufacturer :	Hanna Instruments	Made in :	Romania
Condition As-Received :	Used Product	Reference :	RE240478
Ambient Temperature :	(25 ± 2)°C	Relative Humidity :	(50 ± 15)%RH
Customer name :	United Analyst and Engineering Consultant Co., Ltd. 3 Soi Udomsuk 41, Sukhumvit Rd., Bangchak, Phrakhanong, Bangkok 10260		
Received date :	18 March 2024		
Calibrate date :	18 March 2024		
Issue date :	20 March 2024		
Calibrated Location :	Hanna Instruments (Thailand) Ltd.		
Calibration Procedure :	This calibrator was conducted by using in-house: calibration procedure CP-04 by using certified reference standard instruments.		

Calibrated by :

☒ Mr. Pichit Petthong

☐ Mr. Channarong Soinak

Approved by : 

Mr. Anan Suwanchaisakul
 Authorized Signatory



This certificate was certified only for the instrument we calibrated.
 This result of calibration was found accurate on date and place of calibration only.
 ** This certificate may not be reproduced other than in full, except with the prior written **
 approval of the head of Hanna Instrument (Thailand).

เอกสารไม่ควบคุม

Condition of this calibration result:

Reference Standard Instruments : This certification is traceable to the international unit of unit maintained through:

Instruments	Model	Serial No.	Certificate No.	Traceable
Data Acquisition Switch Unit	34970A	MY44065265	WK2307-164-1	WK Electric Co., Ltd.
Digital Thermo-Hygrometer	HT-771SD	AL07155	24H41	Technology Promotion Association (Thailand-Japan).

Calibration Result:

Measurement Temperature Source Accuracy for COD Reactor.

Capacity (Vial)	Nominal Value (°C)	Average Value (°C)	Uncertainty of Measurement (±°C)
25 Vial	150.0	150.0	0.50

Unit : °C

(1A)	(2A)	(3A)	(4A)	(5A)
150.308	150.221	150.101	150.121	149.738
(1B)	(2B)	(3B)	(4B)	(5B)
150.011	149.395	150.792	149.934	150.178
(1C)	(2C)	(3C)	(4C)	(5C)
150.071	150.052	150.477	150.400	150.451
(1D)	(2D)	(3D)	(4D)	(5D)
149.235	149.601	149.411	150.014	149.708
(1E)	(2E)	(3E)	(4E)	(5E)
150.096	149.107	150.024	150.002	149.342

Figure: Shows the location of the temperature source.

The report uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k=2$, providing a level of confidence of approximately 95%

** End of certificate **

เอกสารไม่ควบคุม

CERTIFICATE OF CALIBRATION

Equipment : COD Test Tube Heater

Meter Model : HI839800-02 **Serial No. :** H0185001

Tube Heater : 25 Vial Capacity **Resolution :** 0.1°C

Temperature Range : (-10 to 160)°C **Temperature of Reaction :** 150°C

Manufacturer : Hanna Instruments **Made in :** Romania

Condition As-Received : Used Product **Reference :** RE250401

Ambient Temperature : (25 ± 2)°C **Relative Humidity :** (50 ± 15)% RH

Customer name : United Analyst and Engineering Consultant Co., Ltd.
3 Soi Udomsuk 41, Sukhumvit Rd., Bangchak,
Phrakhanong, Bangkok 10260

Received date : 5 March 2025


Calibrate date : 7 March 2025

Issue date : 7 March 2025

Calibrated Location : Hanna Instruments (Thailand) Ltd.

Calibration Procedure : This calibrator was conducted by using in-house: calibration procedure CP-04 by using certified reference standard instruments.

Calibrated by : ☒ Mr. Pichit Petthong
☐ Mr. Channarong Soinak

Approved by : 
Mr. Anan Suwanchaisakul
Authorized Signatory



This certificate was certified only for the instrument we calibrated.

This result of calibration was found accurate on date and place of calibration only.

** This certificate may not be reproduced other than in full, except with the prior written **

approval of the head of Hanna Instrument (Thailand).เอกสารไม่ควบคุม

Condition of this calibration result:

Reference Standard Instruments : This certification is traceable to the international unit of unit maintained through:

Instruments	Model	Serial No.	Certificate No.	Traceable
Data Acquisition Switch Unit	34970A	MY44065265	WK2407-141-1	WK Electric Co., Ltd.
Digital Thermo-Hygrometer	HT-771SD	AL07155	25H171	Technology Promotion Association (Thailand-Japan).

Calibration Result:

Measurement Temperature Source Accuracy for COD Reactor.

Capacity (Vial)	Nominal Value (°C)	Average Value (°C)	Uncertainty of Measurement (±°C)
25 Vial	150.0	150.4	0.47

Unit : °C

(1A)	(2A)	(3A)	(4A)	(5A)
150.407	150.377	150.269	150.402	150.422
(1B)	(2B)	(3B)	(4B)	(5B)
150.426	150.394	150.644	150.690	150.542
(1C)	(2C)	(3C)	(4C)	(5C)
150.477	150.303	150.627	150.257	150.176
(1D)	(2D)	(3D)	(4D)	(5D)
150.462	150.456	150.199	150.406	150.102
(1E)	(2E)	(3E)	(4E)	(5E)
150.185	150.513	150.235	150.460	150.442

Figure: Shows the location of the temperature source.

The report uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k=2$, providing a level of confidence of approximately 95%

** End of certificate **

เอกสารไม่ควบคุม

CERTIFICATE OF CALIBRATION

Equipment : COD Test Tube Heater

Meter Model : HI839800-02 **Serial No. :** 04500052101

Tube Heater : 25 Vial Capacity **Resolution :** 0.1°C

Temperature Range : (-10 to 160)°C **Temperature of Reaction :** 150°C

Manufacturer : Hanna Instruments **Made in :** Romania

Condition As-Received : Used Product **Reference :** RE241152

Ambient Temperature : (25 ± 2)°C **Relative Humidity :** (50 ± 15)% RH

Customer name : United Analyst and Engineering Consultant Co., Ltd.
3 Soi Udomsuk 41, Sukhumvit Rd., Bangchak,
Phrakhanong, Bangkok 10260

Received date : 26 June 2024


Calibrate date : 1 July 2024

Issue date : 3 July 2024

Calibrated Location : Hanna Instruments (Thailand) Ltd.

Calibration Procedure : This calibrator was conducted by using in-house: calibration procedure CP-04 by using certified reference standard instruments.

Calibrated by : ☒ Mr. Pichit Petthong
☐ Mr. Channarong Soinak

Approved by : 
Mr. Anan Suwanchaisakul
Authorized Signatory



This certificate was certified only for the instrument we calibrated.

This result of calibration was found accurate on date and place of calibration only.

** This certificate may not be reproduced other than in full, except with the prior written **

approval of the head of Hanna Instrument (Thailand).เอกสารไม่ควบคุม

Condition of this calibration result:

Reference Standard Instruments : This certification is traceable to the international unit of unit maintained through:

Instruments	Model	Serial No.	Certificate No.	Traceable
Data Acquisition Switch Unit	34970A	MY44065265	WK2307-164-1	WK Electric Co., Ltd.
Digital Thermo-Hygrometer	HT-771SD	AL07155	24H41	Technology Promotion Association (Thailand-Japan).

Calibration Result:

Measurement Temperature Source Accuracy for COD Reactor.

Capacity (Vial)	Nominal Value (°C)	Average Value (°C)	Uncertainty of Measurement (±°C)
25 Vial	150.0	149.8	0.48

Unit : °C

(1A)	(2A)	(3A)	(4A)	(5A)
149.574	149.873	149.861	149.748	149.878
(1B)	(2B)	(3B)	(4B)	(5B)
149.490	149.940	149.954	150.103	150.048
(1C)	(2C)	(3C)	(4C)	(5C)
149.625	150.036	150.080	150.015	149.580
(1D)	(2D)	(3D)	(4D)	(5D)
149.801	149.541	149.662	150.010	149.499
(1E)	(2E)	(3E)	(4E)	(5E)
149.563	149.611	149.569	149.831	149.762

Figure: Shows the location of the temperature source.

The report uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k=2$, providing a level of confidence of approximately 95%.

** End of certificate **

เอกสารไม่ควบคุม



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2715-3000-29 FAX. 0-2719-9484



Cert. No.: 24TM589
Page : 1 of 3

Certificate of Calibration

Equipment : Hot Air Oven
Manufacturer : Memmert
Model : UF 55
Serial No. : B212.0411
ID No. : UAE.WAO.005/2556
Submitted by : United Analyst and Engineering Consultant Co.,Ltd.
3 Soi Udomsuk 41, Sukhumvit Road,
Bangchak, Phrakhanong,
Bangkok 10260
Location : Lab Floor 2
Received Order : 01 April 2024
Calibration Date : 01 - 02 April 2024
Ambient Temperature : (26 ± 10) °C
Relative Humidity : (50 ± 30) %
Calibrated by : Krisda Malee
Approved by :
() Ponpan Paipim
(✓) Suwit Imjai
() Kunchit Promprat

Issue Date : 5 April 2024

The Uncertainties are for a confidence probability of approximately 95%.

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

เอกสารไม่ควบคุม
A 0065065

Equipment : Hot Air Oven
Condition As-Received : Used Item
Reference : 2404-0004OC-3
Procedure Used :-

Cert. No.: 24TM589
Page : 2 of 3

Calibration were conducted using calibration procedure CP-OT02 based on TLAS G-20 according to direct measurement method with Data Acquisition which connected with Resistance Temperature Detector (RTD) and Thermocouple Type T.

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

Instrument	Serial No.	Cert. No.	Traceable	Due Date
1) Data Acquisition	MY57013711	23LM115	TPA	11 Jul 2024

2. This certificate is valid only to the item calibrated on date and place of calibration.


3. This certification is traceable to the International System of Unit.

Remark : TPA : Technology Promotion Association (Thailand - Japan)

Result of Calibration :- (*) Without Adjustment

Function of UUC* : Temperature Source

Fresh air setting : Close



Probe Installation Details : Dimension of Chamber :
a = 5.0 cm D = 0.50 m
b = 5.0 cm W = 0.80 m
c = 5.0 cm H = 0.75 m
Capacity = 0.30 m³

Environment during calibration		
	Beginning	Finished
Temp. (°C)	27	26
REL.Humid. (%)	47	48
AC Supply (Volt)	221	220

Ref. Std. ID No.: @ Calibration Point		
Position :	(120 to 180) °C	(104) °C
1	21-18TC-01	22-18RTD-2/1
2	21-18TC-02	18RTD-2/2
3	21-18TC-03	18RTD-2/3
4	21-18TC-04	18RTD-2/4
5	21-18TC-05	18RTD-2/5
6	21-18TC-06	18RTD-2/6
7	21-18TC-07	18RTD-2/7
8	21-18TC-08	18RTD-2/8
9 (ref.)	21-18TC-09	18RTD-2/9

เอกสารไม่ควบคุม
a 1209739

Equipment : Hot Air Oven
Condition As-Received : Used Item
Reference : 2404-0004OC-3
Result of Calibration :- (*) Without Adjustment
Function of UUC* : Temperature Source
Fresh air setting : Close

Cert. No.: 24TM589
Page : 3 of 3

Calibration Point (°C)	UUC* Setting (°C)	UUC* Reading (°C)	Temperature stability (± °C)	Temperature uniformity (°C)	Overall Variation (°C)	Coverage Factor k
104.0	104.0	104.0	0.032	0.47	0.84	2
120.0	120.0	120.0	0.12	0.72	1.3	2
180.0	180.0	180.0	0.13	1.2	1.5	2

Calibration Point (°C)	Measured Temperature (°C)									Uncertainty (± °C)
	1	2	3	4	5	6	7	8	9 (ref.)	
104.0	104.464	103.847	104.236	104.232	104.106	103.691	104.275	104.127	104.013	0.42
120.0	120.486	120.089	120.635	120.596	119.531	119.644	120.364	120.144	120.158	1.1
180.0	180.574	179.769	180.285	180.870	179.594	179.790	180.287	179.961	179.802	1.1

Average* : The average of 30 values in each position.

Temperature stability : One-half of the greatest maximum difference of measured temperature at any one sensor.

Temperature uniformity : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.

Overall Variation : The Difference of the maximum and minimum measured temperatures throughout observation.

UUC* : Unit Under Calibration

Note : The reported uncertainty of measurement was included stability and excluded uniformity .

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k , providing a level of confidence of approximately 95 %.

-o-o-

เอกสารไม่ควบคุม
a 1209738

Certificate of Calibration

Certificate No.: 250422-1-BL002-25

Code No.: BL002-25

Page: 1 of 3

Customer Name: United Analyst and Engineering Consultant Co., Ltd.
Address: 3 Soi Udomsuk 41, Sukhumvit Rd., Bang Chak, Phrakhanong, Bangkok 10260

Equipment: Electronic Balance

Manufacturer: Mettler Toledo

Model: AB204-S/FACT

Serial No.: 1129361010

Asset No.: UAE.WAS.002/2552

Building: N/A **Floor:** 1 **Room:** 107

Received Date: April 22, 2025

Date of Calibration: April 23, 2025

Calibration Conditions: Temperature 22.8 °C to 23.4 °C
Humidity 54.8 % to 68.9 %
Pressure 756.6 mmHg to 758.2 mmHg

Calibrated by: Sakkarin Srirahang

Approved by: Suwit Chotnok

Signature:

Issued Date: April 25, 2025

Note: 1) The Uncertainties are for a confidence probability of approximately 95%

2) This Certificate is valid only to the item calibrated on date and place of calibration.

3) This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the United Analyst and Engineering Consultant Co., Ltd. (UAE)

เอกสารไม่ควบคุม

Certificate No.: 250422-1-BL002-25

Code No.: BL002-25

Page: 2 of 3

Equipment: Electronic Balance

Model: AB204-S/FACT

Serial No.: 1129361010

Max. Capacity: 220 g

Calibration Date: April 23, 2025

Condition As-Received: In Condition

Manufacturer: Mettler Toledo

Readability: 0.0001 g

ID No.: UAE.WAS.002/2552

Condition of Equipment:

Condition of This Result of Calibration:

1. Calibration Method: This instrument was calibrated by method UAE-CP-CAL-006 In-House Method based on UKAS Lab 14 : 2022

2. Reference Standards:

Reference Standard:	Model	Serial No.	Calibrated By	Certificate No.	Traceability	Due Date
Standard Weight Class E2 (OIML)	1 mg to 1 kg	8749109122	AMARC	25-009359	Mettler-Toledo	21-Jan-27
Standard Weight Class F1 (OIML)	1 mg to 200 g	11119512	AMARC	24-013840	Mettler-Toledo	04-Feb-26
Instrument	Model	Serial No.	Calibrated By	Certificate No.	Traceability	Due Date
Thermo-Hydro-Baro Meter	MHB-3825D	AK.6645T	SUCCESS	SG-H-00997/67	Success Gateway	21-Nov-25
Thermo-Hydro-Baro Meter	MHB-3825D	AK.6645T	TPA	25PT95	TPA	25-Feb-26

3. This certification is traceable to SI Unit

4. This certification was certified only for the instrument we calibrated

5. This result of calibration was found accurate as shown on date and place of calibration only.

6. Through the reference standard laboratory of AMARC 25-009359 Calibration 0152

Calibration Result:


1. Repeatability of Reading:

Nominal Value (g)	Standard Deviation of Reading (g)
200*	0.000045

2. Eccentric or off-center loading

A mass of 100 g was placed and moved to various positions on pan

The Balance reading obtained is given in the table.



1 (g)	2 (g)	3 (g)	4 (g)	5 (g)	Maximum Difference (g)
100.0000	99.9996	99.9997	100.0003	100.0005	0.0005

เอกสารไม่ควบคุม

Certificate No.: 250422-1-BL002-25

Code No.: BL002-25

Page: 3 of 3

Equipment: Electronic Balance

Model: AB204-S/FACT

Serial No.: 1129361010

Max. Capacity: 220 g

Calibration Date: April 23, 2025

Calibration Result: (Continued)

Calibration Range: 0 - 200 g

Calibration Adjustment: Internal Calibration

3. Error of indication from nominal or conventional mass value:

Nominal Value (g)	Reference Value (g)	Indication (g)	Correction (g)	Uncertainty (± mg)	Coverage Factor k
Unload	0.0000000	0.0000	0.0000	0.10	2.05
0.01	0.0100025	0.0099	0.0001	0.10	2.05
0.05	0.0500056	0.0500	0.0000	0.10	2.05
0.1	0.1000012	0.0999	0.0001	0.10	2.05
0.5	0.5000133	0.5000	0.0000	0.10	2.05
1	1.0000165	1.0000	0.0000	0.10	2.05
10	10.000010	10.0000	0.0000	0.11	2.04
40	40.000076	40.0000	0.0000	0.14	2.00
50	50.000056	50.0000	0.0001	0.13	2.00
80	80.000107	80.0000	0.0001	0.18	2.00
100	100.000109	99.9999	0.0002	0.17	2.00
120	120.00015	119.9999	0.0003	0.21	2.00
150	150.000165	149.9998	0.0003	0.24	2.00
160	160.000175	159.9997	0.0005	0.26	2.00
200	200.000129	199.9998	0.0004	0.30	2.00

4. Effect of Tare test:

Tare Load (g)	Test Load (g)	Indication (g)	Correction (g)
100	20.000041	19.9999	0.0001
	40.000076	39.9998	0.0002
	60.000066	59.9997	0.0003
	80.000107	79.9999	0.0002
	100.000168	100.0004	-0.0003

Remark:

The report uncertainty of measurement was based on standard uncertainty multiplied by coverage factor k, providing

เอกสารไม่ควบคุม

o--o-End-o--o



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000-29 FAX. 0-2719-9484



Certificate of Calibration

Cert. No.: 24TM647

Page: 1 of 3

Equipment: Incubator

Manufacturer: Binder

Model: KB 400 E6

Serial No.: 2020000015535

ID No.: UAE.MIC.018/2564

Submitted by: United Analyst and Engineering Consultant Co., Ltd.
3 Soi Udomsuk 41, Sukhumvit Road,
Bangchak, Phrakhanong,
Bangkok 10260

Location: Microbiology Laboratory (302)

Received Order: 01 April 2024

Calibration Date: 01 April 2024

Ambient Temperature: (26 ± 10) °C

Relative Humidity: (50 ± 30) %

Calibrated by: Man Pattanapongpaiboon

Approved by:

() Ponpan Paipim
(✓) Suwit Imjai
() Kunchit Promprat

Approved Signatory

Issue Date:

7 April 2024

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written approval of the head of Corporate Services 3: Equipment Calibration and Testing Services.

เอกสารไม่ควบคุม



Equipment : Incubator
Condition As-Received : Used Item
Reference : 2404-0003OC-6
Procedure Used :-

Cert. No.: 24TM647
Page : 2 of 3

Calibration were conducted using calibration procedure CP-OT02 based on TLAS G-20 according to direct measurement method with Data Acquisition which connected with Resistance Temperature Detector (RTD).
The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

Instrument Serial No. Cert. No. Traceable Due Date
1) Data Acquisition MY49023932 23LM122 TPA 26 Jul 2024


2. This certificate is valid only to the item calibrated on date and place of calibration.
3. This certification is traceable to the International System of Unit.

Remark : TPA : Technology Promotion Association (Thailand - Japan)

Result of Calibration :- (*) Without Adjustment

Function of UUC* : Temperature Source

Fresh air setting : Close



Probe Installation Details :

a = 10 cm
b = 10 cm
c = 10 cm

Dimension of Chamber :

D = 0.48 m
W = 0.65 m
H = 1.2 m
Capacity = 0.37 m³

Environment during calibration		
	Beginning	Finished
Temp. (°C)	24	24
REL.Humid. (%)	54	57
AC Supply (Volt)	221	223

Position :	Ref. Std. ID No.:
1	20-16RTD-01
2	20-16RTD-02
3	20-16RTD-03
4	23-16RTD-04
5	22-16RTD-05
6	20-16RTD-06
7	20-16RTD-07
8	22-16RTD-08
9 (ref.)	22-16RTD-09



Equipment : Incubator
Condition As-Received : Used Item
Reference : 2404-0003OC-6
Result of Calibration :- (*) Without Adjustment
Function of UUC* : Temperature Source
Fresh air setting : Close

Cert. No.: 24TM647
Page : 3 of 3

Calibration Point (°C)	UUC* Setting (°C)	UUC* Reading (°C)	Temperature stability (± °C)	Temperature uniformity (°C)	Overall Variation (°C)	Coverage Factor k
35.0	35.0	35.0	0.035	0.19	0.22	2

Calibration Point (°C)	Measured Temperature (°C)									Uncertainty (± °C)
	1	2	3	4	5	6	7	8	9 (ref.)	
35.0	35.000	35.022	34.841	34.851	35.027	35.011	35.023	35.028	35.007	0.30

Average* : The average of 30 values in each position.

Temperature stability : One-half of the greatest maximum difference of measured temperature at any one sensor.

Temperature uniformity : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.

Overall Variation : The Difference of the maximum and minimum measured temperatures throughout observation.

UUC* : Unit Under Calibration

Note : The reported uncertainty of measurement was included stability and excluded uniformity .

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k, providing a level of confidence of approximately 95 %.

-o0o-

เอกสารไม่ควบคุม

เอกสารไม่ควบคุม



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL.0-2717-3000-29 FAX.0-2719-9484



Certificate of Calibration

Cert. No.: 24TM938
Page : 1 of 3

Equipment : Incubator

Manufacturer : Binder

Model : KB 400 E6

Serial No. : 2022000022479

ID No. : UAE.MIC.028/2566

Submitted by : United Analyst and Engineering Consultant Co.,Ltd.
3 Soi Udomsuk 41, Sukhumvit Road,
Bangchak, Phrakhanong,
Bangkok 10260

Location : Microbiology Laboratory

Received Order : 09 July 2024

Calibration Date : 09 July 2024

Ambient Temperature : (26 ± 10) °C

Relative Humidity : (50 ± 30) %

Calibrated by : Khit Ruttanaprapachai

Approved by :

() Ponpan Paipim
(✓) Suwit Injai
() Kunchit Promprat

Issue Date : 19 July 2024

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written Approval of the head of Corporate Services 3: Equipment Calibration and Testing Services.

เอกสารไม่ควบคุม



Equipment : Incubator
Condition As-Received : Used Item
Reference : 2407-0153OC-4

Cert. No.: 24TM938
Page : 2 of 3

Procedure Used :-

Calibration were conducted using calibration procedure CP-OT02 based on TLAS G-20 according to direct measurement method with Data Acquisition which connected with Resistance Temperature Detector (RTD).
The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

Instrument Serial No. Cert. No. Traceable Due Date
1) Data Acquisition MY49001451 24LM44 TPA 17 Mar 2025

2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certification is traceable to the International System of Unit.


Remark : TPA : Technology Promotion Association (Thailand - Japan)

Result of Calibration :- (*) Without Adjustment

Function of UUC* : Temperature Source

Fresh air setting : Not Available

Environment during calibration		
	Beginning	Finished
Temp. (°C)	23	24
REL.Humid. (%)	52	54
AC Supply (Volt)	221	222



Probe Installation Details :

a = 10 cm
b = 10 cm
c = 10 cm

Dimension of Chamber :

D = 0.47 m
W = 0.65 m
H = 1.2 m
Capacity = 0.37 m³

Position :	Ref. Std. ID No.:
1	19RTD-2/1
2	19RTD-2/2
3	19RTD-2/3
4	19RTD-2/4
5	19RTD-2/5
6	24-19RTD-2/6
7	19RTD-2/7
8	19RTD-2/8
9 (ref.)	19RTD-2/9

เอกสารไม่ควบคุม



Equipment : Incubator
Condition As-Received : Used Item
Reference : 2407-0153OC-4
Result of Calibration :- (*) Without Adjustment
Function of UUC* : Temperature Source
Fresh air setting : Not Available

Cert. No.: 24TM938
Page : 3 of 3

Calibration Point (°C)	UUC* Setting (°C)	UUC* Reading (°C)	Temperature stability (± °C)	Temperature uniformity (°C)	Overall Variation (°C)	Coverage Factor k
35.0	35.0	35.0	0.030	0.31	0.33	2

Calibration Point (°C)	Measured Temperature (°C)									Uncertainty (± °C)
	Position									
	1	2	3	4	5	6	7	8	9 (ref.)	
35.0	35.093	35.011	35.081	35.118	34.840	35.054	34.924	34.978	34.824	0.30

Average* : The average of 30 values in each position.
Temperature stability : One-half of the greatest maximum difference of measured temperature at any one sensor.
Temperature uniformity : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.
Overall Variation : The Difference of the maximum and minimum measured temperatures throughout observation.
UUC* : Unit Under Calibration
Note : The reported uncertainty of measurement was included stability and excluded uniformity .

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k, providing a level of confidence of approximately 95 %.

-o0o-

เอกสารไม่ควบคุม



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL.0-2717-3000-29 FAX.0-2719-9484



Certificate of Calibration

Cert. No.: 24TM884
Page : 1 of 3

Equipment : Incubator
Manufacturer : Binder
Model : KB 400
Serial No. : 20220000000391
ID No. : UAE.MIC.029/2565
Submitted by : United Analyst and Engineering Consultant Co.,Ltd.
3 Soi Udomsuk 41, Sukhumvit Road,
Bangchak, Phrakhanong,
Bangkok 10260
Location : Microbiology Laboratory
Received Order : 07 June 2024
Calibration Date : 07 June 2024
Ambient Temperature : (26 ± 10) °C
Relative Humidity : (50 ± 30) %
Calibrated by : Tawatchai Pama
Approved by : Kunchit
() Ponpan Paipim
() Suwit Imjai
(✓) Kunchit Promprat

Issue Date : 11 June 2024

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written Approval of the head of Corporate Services 3: Equipment Calibration and Testing Services.

เอกสารไม่ควบคุม



Equipment : Incubator
Condition As-Received : Used Item
Reference : 2406-0190OC-2

Cert. No.: 24TM884
Page : 2 of 3

Procedure Used :-

Calibration were conducted using calibration procedure CP-OT02 based on TLAS G-20 according to direct measurement method with Data Acquisition which connected with Resistance Temperature Detector (RTD).
The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

Instrument	Serial No.	Cert. No.	Traceable	Due Date
1) Data Acquisition	MY49001451	24LM44	TPA	17 Mar 2025


2. This certificate is valid only to the item calibrated on date and place of calibration.
3. This certification is traceable to the International System of Unit.

Remark : TPA : Technology Promotion Association (Thailand - Japan)

Result of Calibration :- (*) Without Adjustment

Function of UUC* : Temperature Source

Fresh air setting : Close



Probe Installation Details :

a = 10 cm
b = 10 cm
c = 10 cm

Dimension of Chamber :

D = 0.50 m
W = 0.65 m
H = 1.2 m
Capacity = 0.39 m³

Environment during calibration		
	Beginning	Finished
Temp. (°C)	21	19
REL.Humid. (%)	77	75
AC Supply (Volt)	228	229

Position :	Ref. Std. ID No.:
1	19RTD-2/1
2	19RTD-2/2
3	19RTD-2/3
4	19RTD-2/4
5	19RTD-2/5
6	24-19RTD-2/6
7	19RTD-2/7
8	19RTD-2/8
9 (ref.)	19RTD-2/9

-o0o-

เอกสารไม่ควบคุม



Equipment : Incubator
Condition As-Received : Used Item
Reference : 2406-0190OC-2
Result of Calibration :- (*) Without Adjustment
Function of UUC* : Temperature Source
Fresh air setting : Close

Cert. No.: 24TM884
Page : 3 of 3

Calibration Point (°C)	UUC* Setting (°C)	UUC* Reading (°C)	Temperature stability (± °C)	Temperature uniformity (°C)	Overall Variation (°C)	Coverage Factor k
35.0	35.0	35.0	0.028	0.28	0.53	2

Calibration Point (°C)	Measured Temperature (°C)									Uncertainty (± °C)
	Position									
	1	2	3	4	5	6	7	8	9 (ref.)	
35.0	35.317	35.184	35.142	35.064	35.098	35.093	34.894	34.826	35.056	0.30

Average* : The average of 30 values in each position.
Temperature stability : One-half of the greatest maximum difference of measured temperature at any one sensor.
Temperature uniformity : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.
Overall Variation : The Difference of the maximum and minimum measured temperatures throughout observation.
UUC* : Unit Under Calibration
Note : The reported uncertainty of measurement was included stability and excluded uniformity .

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k, providing a level of confidence of approximately 95 %.

-o0o-

เอกสารไม่ควบคุม

กำหนดจุดห้ามใช้งาน

References Certificate Number. : 24TM884

Equipment : Incubator

Model : KB 400


Serial No. : 20220000000391

ID No. : UAE.MIC.029/2565

Manufacturer : Binder

Calibration Point : 35.0 °C

Unit Under Calibration Setting : 35.0 °C

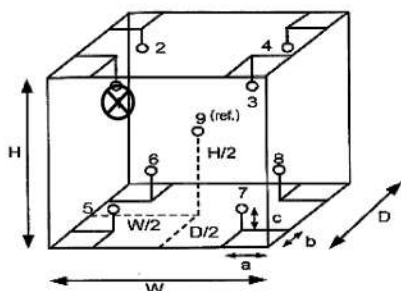

รูปภาพเครื่องมือ แสดงจุดที่ได้รับการสอบเทียบ และสัญลักษณ์ ⊗ แสดงจุดห้ามใช้งาน

กำหนดจุดห้ามใช้งานตำแหน่งที่.....1.....

หมายเหตุ เก็บใบแนบ.....

\\uae-netapp\Netapp_LAB\Lab-3\INSTRUMENT\01-2024\FCertificate\เข้างาน\งานสอบเทียบ\งานสอบเทียบ 2565\กำหนดจุดห้ามใช้งาน\กำหนดจุดห้ามใช้งาน 1

เอกสารไม่ควบคุม

FOSS

FOSS South East Asia
3388 Sirinrat Building, 25th - 26th Floor, Unit No. 3388/90,
Rama IV Road, Klongton, Klongtoey, Bangkok, Thailand 10110

Customer Service Report

Report No.: 12875

Date: July 5, 2024

Customer: UAE

Job No.: 8315

Address: Bangkok

Instrument: KT9 Distilator

Serial: 91405393

Travel To Customer (Hrs)	Labour (Hrs)	Travel From Customer (Hrs)
08.30 - 14.30	09.30 - 14.30	14.30 - 16.00
1	5	1.5

Application	Special	Standard
Distributor	Courtesy Visit	Installation
Digital Service	PMA Onboarding	Quote
Internal	Warranty	Repair
Investigate	Sales Support	Remote
		Health Check Visit

PMA Type	Smartcare	x	Smartcare Pro	x	Fosscore	
	Smartcare Advance	x	Fosscore Pro	x	N/A	x

Details of Work / Test
- PM -
- Visual Check -
+ No leak
+ No drawing
- Change PM kit x1 set -ok
- Function Check -
+ Dilution 80 mL → 50 mL
+ Alkali 50 mL → 50 mL
+ Receiver N/A → Notice
+ Hecm / Drain
Blank = Follow up, Recovery = 100% SP = Follow up
Instrument Ready for Use
OK
Not OK*

Part No.	Batch	Description	Qty
60100146	03-01-2024	PM kit Bjeltec 9 Distilator	1

Signed FOSS	Signed Customer
Name	Name

Email: Customer Contact: *

*Remark:

เอกสารไม่ควบคุม

TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000-29 FAX. 0-2719-9484Cert.No.: 24CH400
Page: 1 of 3

Certificate of Calibration

Equipment : pH Meter
Manufacturer : Horiba
Model : LAQUA-PH210
Serial No. : HA9M0047
ID No. : UAE.EFM.005/2563(EFM.pH.05/63)
Condition As-Received: Used Item
Received Date : 01 April 2024
Calibration Date : 02 April 2024
Reference : 2404-0037WSC-2
Submitted by : United Analyst and Engineering Consultant Co.,Ltd.
3 Soi Udomsuk 41, Sukhumvit Road,
Bangchak, Phrakhanong, Bangkok 10260

Ambient Temperature : (25 ± 2.5) °C
Relative Humidity : (50 ± 15) %
Calibration Procedure : In - house method :
- CP-CH5 by direct measurement with DC voltage standard and direct measurement with certified reference material (CRM)
- CP-CH8 by comparison with temperature standard

Calibrated by : Warakorn Lemgagrakul

Approved by : Approved Signatory

() Pornthippa Tameyakul
() Unnopphol Harachai
(✓) Salthip Meangmai

Issue Date : 06 April 2024

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 - Equipment Calibration and Testing Services.

Cert.No.: 24CH400
Page: 2 of 3

Condition of this calibration result

1. Reference Standard Instrument

Instrument	Serial No.	ID No.	Cert. No.	Due Date
1) Document Process Calibrator	54030049	130RC116	23E2802	27 Aug 2024
2) Ref. Standard Thermometer	4982054	110RC044	23I908	26 July 2024

This certification is traceable to the International System of Unit maintained through:-
- Technology Promotion Association (Thailand-Japan)

2. Certified Reference Materials : The measurement results are traceable to SI through CPA chem Ltd.,
ANSI-ASQ National Accreditation Board, Accredited No. AR-1835

Buffer Solution	Manufacturer	Lot No.	Exp. date
pH 4.008	CPA chem	940102	27 Nov 2025
pH 6.986	CPA chem	940104	02 Nov 2024
pH 9.997	CPA chem	940106	02 Nov 2024

3. This certificate is valid only to the item calibrated on date and place of calibration.

Calibration Results

Function : mV Measurement

Performing standard curve by Document Process Calibrator at pH (4,7)(7,10)

Unit Under Calibration	Nominal Value	Standard Voltage Input	Actual Reading	Uncertainty of Measurement	Coverage factor
	pH	mV	mV	(± mV)	k
pH Meter	4.00	177.48	177.3	0.058	2.00
S/N.: HA9M0047	7.00	0.00	0.0	0.058	2.00
	7.00	0.00	0.0	0.058	2.00
	10.00	-177.48	-177.4	0.058	2.00

Salthip



Cert.No.: 24CH400
Page.: 3 of 3

Calibration Results

Function : pH Measurement

Performing three buffers standard curve by using buffer nominal pH (4,7)(7,10)

Unit Under Calibration	Standard pH Buffer Solution	Actual pH Reading	Actual mV Reading (mV)	Uncertainty of pH Measurement (\pm)	Coverage factor k
pH Electrode S/N.: -	4.008	4.01	171.5	0.0079	2.00
	6.986	6.99	-8.4	0.0099	2.00
	6.986	7.00	-9.6	0.011	2.00
	9.997	10.02	-173.8	0.0096	2.00

Function : Temperature Measurement

(*) Without adjustment

This equipment was connected with Temperature Probe;

- Model : -
- Serial No. : -
Dimension of probe
- Length : 103 mm.
- Diameter : 16 mm.
- Immersion Depth : 90 mm.

Calibration Point ($^{\circ}\text{C}$)	Standard Temperature ($^{\circ}\text{C}$)	UUC* Reading ($^{\circ}\text{C}$)	Error ($^{\circ}\text{C}$)	Uncertainty of measurement (\pm $^{\circ}\text{C}$)	Coverage factor k
25.0	25.002	25.0	-0.002	0.13	2.00
30.0	30.002	30.0	-0.002	0.13	2.00
35.0	35.003	35.0	-0.003	0.13	2.00

Remark : - UUC* = Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k , providing a level of confidence of approximately 95 %.

-00o-

a 1209884



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD S/DI 18, SUANLIANG, SUANLIANG BANGKOK 10250
TEL.0-2717-3000-29 FAX.0-2719-9484



Certificate of Calibration

Cert.No.: 25CH354
Page.: 1 of 3

Equipment : pH Meter
Manufacturer : Horiba
Model : LAQUA-PH210
Serial No. : HA9M0047
ID No. : UAE.EFM.005/2563 (EFM.pH.05/63)
Condition As-Received: Used Item
Received Date : 18 March 2025
Calibration Date : 20 March 2025
Reference : 2503-0612WSC-2
Submitted by : United Analyst and Engineering Consultant Co.,Ltd.
3 Soi Udomsuk 41, Sukhumvit Road, Bangchak,
Phrakhanong, Bangkok 10260

Ambient Temperature : (25 \pm 2.5) $^{\circ}\text{C}$
Relative Humidity : (50 \pm 15) %
Calibration Procedure : In - house method :
- CP-CH5 by direct measurement with DC voltage standard and direct measurement with certified reference material (CRM)
- CP-CH8 by comparison with temperature standard

Calibrated by : Uthen Kankawi

Approved by : Approved Signatory

() Chakrit Waewwanjua
() Nonpan Paipim
(✓) Saitip Meangmai

Issue Date : 20 March 2025

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written Approval of the head of Corporate Services 3: Equipment Calibration and Testing Services.



Cert.No.: 25CH354
Page.: 2 of 3

Condition of this calibration result

1. Reference Standard Instrument

Instrument	Serial No.	ID No.	Cert. No.	Due Date
1) Document Process Calibrator	43160066	130RC092	24E1320	22 Apr 2025
2) Ref. Standard Thermometer	4982054	110RC044	24I757	14 Jul 2025

- This Certification is traceable to SI Through Technology Promotion Association (Thailand - Japan)

2. Certified Reference Materials :The measurement results are traceable to SI through Hach Lenge GmbH Ltd.,
Deutsche Akkreditierungsstelle, Accredited No.D-RM-15184-01-00
: The measurement results are traceable to SI through CPA chem Ltd.,
ANSI-ASQ National Accreditation Board, Accredited No. AR-1835

Buffer Solution	Manufacturer	Lot No.	Exp. date
pH 4.007	CPA chem	1066665	18 Jan 2027
pH 6.999	Hach Lenge GmbH	C03220	29 Oct 2026
pH 10.010	CPA chem	1066669	18 Jan 2026

3. This certificate is valid only to the item calibrated on date and place of calibration.

Calibration Results

Function : mV Measurement

Performing standard curve by Document Process Calibrator at pH (4,7)(7,10)

Unit Under Calibration	Nominal Value	Standard Voltage Input	Actual Reading		Uncertainty of Measurement (\pm mV)	Coverage factor k
	pH	mV	mV	pH		
pH Meter S/N.: HA9M0047	4.00	177.48	177.7	4.01	0.058	2.00
	7.00	0.00	0.3	7.01	0.058	2.00
	7.00	0.00	0.3	7.01	0.058	2.00
	10.00	-177.48	-176.8	10.01	0.058	2.00

Calibration Results

Function : pH Measurement

Performing three buffers standard curve by using buffer nominal pH (4,7)(7,10)

Unit Under Calibration	Standard pH Buffer Solution	Actual pH Reading	Actual mV Reading (mV)	Uncertainty of pH Measurement (\pm)	Coverage factor k
pH Electrode S/N.: -	4.007	4.01	168.5	0.011	2.13
	6.999	7.00	-5.9	0.012	2.09
	6.999	7.00	-6.1	0.011	2.07
	10.010	10.02	-176.7	0.010	2.00

Function : Temperature Measurement

(*) Without adjustment

This equipment was connected with Temperature Probe;

- Model : -
- Serial No. : -
Dimension of probe
- Length : 103 mm.
- Diameter : 16 mm.
- Immersion Depth : 90 mm.

Calibration Point ($^{\circ}\text{C}$)	Standard Temperature ($^{\circ}\text{C}$)	UUC* Reading ($^{\circ}\text{C}$)	Error ($^{\circ}\text{C}$)	Uncertainty of measurement (\pm $^{\circ}\text{C}$)	Coverage factor k
15.0	15.005	15.0	-0.005	0.13	2.00
30.0	30.007	30.0	-0.007	0.13	2.00
45.0	44.995	44.9	-0.095	0.13	2.00

Remark : - UUC* = Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k , providing a level of confidence of approximately 95 %.

-00o-

Certificate of Calibration

Cert.No.: 25CH262
Page.: 1 of 3

Equipment :	pH Meter
Manufacturer :	Horiba
Model :	LAQUA-PH210
Serial No. :	HA1L0035
ID No. :	UAE,EFM.011/2565(EFM,pH.01/65)
Condition As-Received:	Used Item
Received Date :	25 February 2025
Calibration Date :	26 to 28 February 2025
Reference :	2502-0783WSC-2
Submitted by :	United Analyst and Engineering Consultant Co.,Ltd, 3 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260

Ambient Temperature :	(25 ± 2.5) °C
Relative Humidity :	(50 ± 15) %
Calibration Procedure :	In - house method : <ul style="list-style-type: none"> - CP-CH5 by direct measurement with DC voltage standard and direct measurement with certified reference material (CRM) - CP-CH8 by comparison with temperature standard

Calibrated by : Warakorn Lerngagtrakul

Approved by : _____
Approved Signatory

() Chakrit Waewwanjua
() Ponpan Paipim
(✓) Saithip Meangmai

Issue Date : 28 February 2025

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.



Cert.No.: 25CH262
Page.: 2 of 3

Condition of this calibration result

1. Reference Standard Instrument

<u>Instrument</u>	<u>Serial No.</u>	<u>ID No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
1)Document Process Calibrator	54030049	130RC116	24E2759	25 Aug 2025
2)Ref. Standard Thermometer	4982054	110RC044	24I757	14 July 2025

- This Certification is traceable to SI Throught Technology Promotion Association (Thailand - Japan)

2. Certified Reference Materials :The measurement results are traceable to SI through Hach Lenge GmbH Ltd., Deutsche Akkreditierungsstelle, Accredited No.D-RM-15184-01-00
: The measurement results are traceable to SI through CPA chem Ltd., ANSI-ASQ National Accreditation Board, Accredited No. AR-1835

<u>Buffer Solution</u>	<u>Manufacturer</u>	<u>Lot No.</u>	<u>Exp. date</u>
pH 4.007	CPA chem	1066665	18 Jan 2027
pH 6.999	Hach Lenge GmbH	C03220	29 Oct 2026
pH 10.010	CPA chem	1066669	18 Jan 2026

3. This certificate is valid only to the item calibrated on date and place of calibration.

Calibration Results

Function : mV Measurement

Performing standard curve by Document Process Calibrator at pH (4,7)(7,10)

Unit Under Calibration	Nominal Value	Standard Voltage Input	Actual Reading		Uncertainty of Measurement	Coverage factor
	pH	mV	mV	pH	(\pm mV)	k
pH Meter	4.00	177.48	177.5	4.01	0.058	2.00
S/N.: HA1L0035	7.00	0.00	0.1	7.02	0.058	2.00
	10.00	0.00	0.1	7.02	0.058	2.00
	10.00	-177.48	-177.4	10.01	0.329	4.53



Cert.No.: 25CH262
Page.: 3 of 3

Calibration Results

Function : pH Measurement

Performing three buffers standard curve by using buffer nominal pH (4,7)(7,10)

Unit Under Calibration	Standard pH Buffer Solution	Actual pH Reading	Actual mV Reading (mV)	Uncertainty of pH Measurement (\pm)	Coverage factor k
pH Electrode	4.007	4.01	178.3	0.0085	2.05
S/N.: -	6.999	7.00	2.3	0.0092	2.00
	6.999	7.00	2.4	0.0092	2.00
	10.010	10.01	-172.2	0.0092	2.00

Function : Temperature Measurement

(*) Without adjustment

This equipment was connected with Temperature Probe;

- Model : -

- Serial No. : _____ -

Dimension of probe

- Length : 110 mm.

- Diameter : 16 mm.

- Immersion Depth : 80 mm.

Calibration Point (°C)	Standard Temperature (°C)	UUC* Reading (°C)	Error (°C)	Uncertainty of measurement (± °C)	Coverage factor k
15.0	15,003	15.0	-0.003	0.13	2.00
30.0	30,004	30.0	-0.004	0.13	2.00
45.0	45.002	45.0	-0.002	0.13	2.00

Remark - $UUC^* = \text{Unit Under Calibration}$

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k , providing a level of confidence of approximately 95 %.

Certificate of Calibration

Cert.No.: 25CH263
Page.: 1 of 3

Equipment :	pH Meter
Manufacturer :	Horiba
Model :	LAQUA-PH210
Serial No. :	HA1M0043
ID No. :	UAE,EFM.013/2565(EFM,pH.03/65)
Condition As-Received:	Used Item
Received Date :	25 February 2025
Calibration Date :	26 to 28 February 2025
Reference :	2502-0783WSC-3
Submitted by :	United Analyst and Engineering Consultant Co.,Ltd. 3 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260

Ambient Temperature :	(25 ± 2.5) °C
Relative Humidity :	(50 ± 15) %
Calibration Procedure :	In - house method : - CP-CH5 by direct measurement with DC voltage standard and direct measurement with certified reference material (CRM) - CP-CH8 by comparison with temperature standard

Calibrated by : Warakorn Lemgagtrakul

Approved by : _____
Approved Signatory

() Chakrit Waewwanjua
() Ponpan Paipim
(✓) Saithip Meangmai

Issue Date : 28 February 2025

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.



Cert.No.: 25CH263
Page.: 2 of 3

Condition of this calibration result

1. Reference Standard Instrument

<u>Instrument</u>	<u>Serial No.</u>	<u>ID No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
1) Document Process Calibrator	54030049	130RC116	24E2759	25 Aug 202
2) Ref. Standard Thermometer	4982054	110RC044	24I757	14 July 202

- This Certification is traceable to SI Throught Technology Promotion Association (Thailand - Japan)

2. Certified Reference Materials :The measurement results are traceable to SI through Hach Lenge GmbH Ltd., Deutsche Akkreditierungsstelle, Accredited No.D-RM-15184-01-00
: The measurement results are traceable to SI through CPA chem Ltd., ANSI-ASQ National Accreditation Board, Accredited No. AR-1835

<u>Buffer Solution</u>	<u>Manufacturer</u>	<u>Lot No.</u>	<u>Exp. date</u>
pH 4.007	CPA chem	1066665	18 Jan 2027
pH 6.999	Hach Lenge GmbH	C03220	29 Oct 2026
pH 10.010	CPA chem	1066669	18 Jan 2026

3. This certificate is valid only to the item calibrated on date and place of calibration.

Calibration Results

Function : mV Measurement

Performing standard curve by Document Process Calibrator at pH (4,7)(7,10)

Unit Under Calibration	Nominal Value	Standard Voltage Input	Actual Reading		Uncertainty of Measurement	Coverage factor
	pH	mV	mV	pH	($\pm mV$)	k
pH Meter	4.00	177.48	177.4	4.01	0.058	2.00
S/N.: HA1M0043	7.00	0.00	-0.1	7.00	0.058	2.00
	7.00	0.00	-0.1	7.00	0.058	2.00
	10.00	-177.48	-177.6	10.01	0.058	2.00



Cert.No.: 25CH263
Page.: 3 of 3

Calibration Results

Function : pH Measurement

Performing three buffers standard curve by using buffer nominal pH (4,7)(7,10)

Unit Under Calibration	Standard pH Buffer Solution	Actual pH Reading	Actual mV Reading (mV)	Uncertainty of pH Measurement (\pm)	Coverage factor k
pH Electrode S/N.: 992H0385	4.007	4.01	147.9	0.0085	2.05
	6.999	7.00	-24.3	0.0092	2.00
	6.999	7.01	-24.4	0.0085	2.00
	10.010	10.01	-197.8	0.0092	2.00

Function : Temperature Measurement

(*) Without adjustment

This equipment was connected with Temperature Probe;

- Model : 9652

- Serial No. : 992H0385

Dimension of probe

- Length : 110 mm

- Diameter : 16 mm

- Immersion Depth : 80 mm.

--	--

Calibration Point (°C)	Standard Temperature (°C)	UUC* Reading (°C)	Error (°C)	Uncertainty of measurement (± °C)	Coverage factor <i>k</i>
15.0	15.003	15.0	-0.003	0.13	2.00
30.0	30.004	30.0	-0.004	0.13	2.00
45.0	45.002	45.0	-0.002	0.13	2.00

Remark - UUC* = Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k , providing a level of confidence of approximately 95 %.



Certificate of Calibration

Cert.No.: 24CH726
Page.: 1 of 3

Equipment : pH Meter
Manufacturer : Horiba
Model : LAQUA-PH210
Serial No. : HA0E0006
ID No. : UAE EFM.070/2564(EFM.pH.03/64)
Condition As-Received: Used Item
Received Date : 18 June 2024
Calibration Date : 19 June 2024
Reference : 2406-0570WSC-4
Submitted by : United Analyst and Engineering Consultant Co.,Ltd.
3 Soi Udomsuk 41, Sukhumvit Road,
Bangchak, Phrakhanong, Bangkok 10260

Ambient Temperature : (25 ± 2.5) °C
Relative Humidity : (50 ± 15) %
Calibration Procedure : In - house method :
- CP-CH5 by direct measurement with DC voltage
standard and direct measurement with
certified reference material (CRM)
- CP-CH8 by comparison with temperature standard

Calibrated by : Warakorn Lernagatrakul

Approved by :

Saithip
Approved Signatory

() Unnopphol Harachai
() Ponpan Paipim
(✓) Saithip Meangmai

Issue Date : 20 June 2024

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

Condition of this calibration result

Instrument	Serial No.	ID No.	Cert. No.	Due Date
1) Document Process Calibrator	54030049	130RC116	23E2802	27 Aug 2024
2) Ref. Standard Thermometer	4982054	110RC044	23/908	26 July 2024

- This Certification is traceable to SI Through Technology Promotion Association (Thailand - Japan)

2. Certified Reference Materials : The measurement results are traceable to SI through CPA chem Ltd.,
ANSI-ASQ National Accreditation Board, Accredited No. AR-1835

Buffer Solution	Manufacturer	Lot No.	Exp. date
pH 4.008	CPA chem	970851	25 Apr 2026
pH 6.986	CPA chem	970852	25 Apr 2025
pH 9.997	CPA chem	970853	25 Apr 2025

3. This certificate is valid only to the item calibrated on date and place of calibration.

Calibration Results

Function : mV Measurement

Performing standard curve by Document Process Calibrator at pH (4.7)(7,10)

Unit Under Calibration	Nominal Value	Standard Voltage Input	Actual Reading		Uncertainty of Measurement	Coverage factor
	pH	mV	mV	pH	(±mV)	k
pH Meter S/N.: HA0E0006	4.00	177.48	177.5	4.01	0.058	2.00
	7.00	0.00	0.1	7.00	0.058	2.00
	7.00	0.00	0.1	7.00	0.058	2.00
	10.00	-177.48	-177.4	10.01	0.058	2.00



Cert.No.: 24CH726
Page.: 3 of 3

Calibration Results

Function : pH Measurement

Performing three buffers standard curve by using buffer nominal pH (4.7)(7,10)

Unit Under Calibration	Standard pH Buffer Solution	Actual pH Reading	Actual mV Reading (mV)	Uncertainty of pH Measurement (±)	Coverage factor k
pH Electrode S/N.: Q9AD0140	4.008	4.01	174.6	0.0079	2.00
	6.986	6.99	-0.8	0.0093	2.00
	6.986	7.00	-0.9	0.0093	2.00
	9.997	10.01	-175.6	0.0095	2.00

Function : Temperature Measurement

(*) Without adjustment

This equipment was connected with Temperature Probe;

- Model : 9652-10D
- Serial No. : Q9AD0140

Dimension of probe

- Length : 103 mm.
- Diameter : 16 mm.
- Immersion Depth : 80 mm.

Calibration Point (°C)	Standard Temperature (°C)	UUC* Reading (°C)	Error (°C)	Uncertainty of measurement (± °C)	Coverage factor k
25.0	25.001	25.0	-0.001	0.13	2.00
30.0	30.002	30.0	-0.002	0.13	2.00
35.0	35.002	35.0	-0.002	0.13	2.00

Remark : - UUC* = Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k, providing a level of confidence of approximately 95 %.

-o0o-



Cert.No.: 24CH319
Page.: 1 of 3

Certificate of Calibration

Equipment : pH Meter
Manufacturer : Horiba
Model : LAQUA-PH210
Serial No. : HA0C0025
ID No. : UAE EFM.117/2563(EFM.pH.07/63)
Condition As-Received: Used Item
Received Date : 12 March 2024
Calibration Date : 14 March 2024
Reference : 2403-0386VSC-1
Submitted by : United Analyst and Engineering Consultant Co.,Ltd.
3 Soi Udomsuk 41, Sukhumvit Road,
Bangchak, Phrakhanong, Bangkok 10260

Ambient Temperature : (25 ± 2.5) °C
Relative Humidity : (50 ± 15) %
Calibration Procedure : In - house method :
- CP-CH5 by direct measurement with DC voltage
standard and direct measurement with
certified reference material (CRM)
- CP-CH8 by comparison with temperature standard

Calibrated by : Warakorn Lernagatrakul

Approved by :

Saithip
Approved Signatory

() Pornthippa Tameyakul
() Unnopphol Harachai
(✓) Saithip Meangmai

Issue Date : 15 March 2024

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.



Cert.No.: 24CH319
Page.: 2 of 3

Condition of this calibration result

1. Reference Standard instrument

Instrument	Serial No.	ID No.	Cert. No.	Due Date
1) Document Process Calibrator	54030049	130RC116	23E2802	27 Aug 2024
2) Ref. Standard Thermometer	4982054	110RC044	23I908	26 July 2024

This certification is traceable to the International System of Unit maintained through:-
- Technology Promotion Association (Thailand-Japan)

2. Certified Reference Materials : The measurement results are traceable to SI through CPA chem Ltd.,
ANSI-ASQ National Accreditation Board, Accredited No. AR-1835

Buffer Solution	Manufacturer	Lot No.	Exp. date
pH 4.008	CPA chem	940102	27 Nov 2025
pH 6.986	CPA chem	940104	02 Nov 2024
pH 9.997	CPA chem	940106	02 Nov 2024

3. This certificate is valid only to the item calibrated on date and place of calibration.

Calibration Results

Function : mV Measurement

Performing standard curve by Document Process Calibrator at pH (4,7)(7,10)

Unit Under Calibration	Nominal Value	Standard Voltage Input	Actual Reading		Uncertainty of Measurement	Coverage factor
	pH	mV	mV	pH	(\pm mV)	k
pH Meter S/N.: HAOC0025	4.00	177.48	177.5	4.01	0.058	2.00
	7.00	0.00	0.0	7.02	0.058	2.00
	7.00	0.00	0.0	7.02	0.058	2.00
	10.00	-177.48	-177.5	10.01	0.058	2.00

Saitip

a 1206341



Cert.No.: 24CH319
Page.: 3 of 3

Calibration Results

Function : pH Measurement

Performing three buffers standard curve by using buffer nominal pH (4,7)(7,10)

Unit Under Calibration	Standard pH Buffer Solution	Actual pH Reading	Actual mV Reading (mV)	Uncertainty of pH Measurement (\pm)	Coverage factor k
pH Electrode S/N.: -	4.008	4.01	149.4	0.0091	2.07
	6.986	7.00	-25.1	0.0093	2.00
	6.986	7.02	-24.3	0.011	2.00
	9.997	10.01	-199.5	0.0095	2.00

Function : Temperature Measurement

(*) Without adjustment

This equipment was connected with Temperature Probe;

- Model :	-
- Serial No. :	-
Dimension of probe	
- Length :	103 mm.
- Diameter :	16 mm.
- Immersion Depth :	90 mm.

Calibration Point (°C)	Standard Temperature (°C)	UUC* Reading (°C)	Error (°C)	Uncertainty of measurement (\pm °C)	Coverage factor k
25.0	25.001	25.0	-0.001	0.13	2.00
30.0	30.001	30.0	-0.001	0.13	2.00
35.0	35.002	35.0	-0.002	0.13	2.00

Remark : - UUC* = Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k, providing a level of confidence of approximately 95 %.

-o-o-

Saitip

a 1206342



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL.0-2717-3000-29 FAX.0-2719-9484



Certificate of Calibration

Cert.No.: 24CH1379
Page.: 1 of 3

Equipment : pH Meter
Manufacturer : EcoSense
Model : pH100A
Serial No. : JC03354
ID No. : UAE,EFM,063/2562(ENV,pH03/62)
Condition As-Received: Used Item
Received Date : 05 November 2024
Calibration Date : 06 November 2024
Reference : 2411-0122WSC-1
Submitted by : United Analyst and Engineering Consultant Co.,Ltd,
3 Soi Udomsuk 41, Sukhumvit Road,
Bangchak, Phrakhanong, Bangkok 10260
Ambient Temperature : (25 \pm 2.5) °C
Relative Humidity : (50 \pm 15) %
Calibration Procedure : In - house method :
- CP-CH5 by direct measurement with DC voltage standard and direct measurement with certified reference material (CRM)
- CP-CH8 by comparison with temperature standard
Calibrated by : Warakorn Lemgagtrakul
Approved by :
() Unnopphol Harachai
(✓) Ponpan Paipim
() Saitip Meangmai
Issue Date : 8 November 2024

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written Approval of the head of Corporate Services 3: Equipment Calibration and Testing Services.



Cert.No.: 24CH1379
Page.: 2 of 3

Condition of this calibration result

1. Reference Standard Instrument

Instrument	Serial No.	ID No.	Cert. No.	Due Date
1) Document Process Calibrator	54030049	130RC116	24E2759	25 Aug 2025
2) Ref. Standard Thermometer	4982054	110RC044	24I757	14 July 2025

- This Certification is traceable to SI Through Technology Promotion Association (Thailand - Japan)

2. Certified Reference Materials :The measurement results are traceable to SI through Hach Lenge GmbH Ltd.,
Deutsche Akkreditierungsstelle, Accredited No.D-RM-15184-01-00

Buffer Solution	Manufacturer	Lot No.	Exp. date
pH 4.008	CPA chem	1034203	27 Sep 2026
pH 6.999	Hach Lenge GmbH	C03145	28 Feb 2026
pH 10.010	CPA chem	1034205	27 Sep 2025

3. This certificate is valid only to the item calibrated on date and place of calibration.

Calibration Results

Function : mV Measurement

Performing standard curve by Document Process Calibrator at pH (4,7)(7,10)

Unit Under Calibration	Nominal Value	Standard Voltage Input	Actual Reading		Uncertainty of Measurement	Coverage factor
	pH	mV	mV	pH	(\pm mV)	k
pH Meter S/N.: JC03354	4.00	177.48	177	4.01	0.58	2.00
	7.00	0.00	0	7.00	0.58	2.00
	7.00	0.00	0	7.00	0.58	2.00
	10.00	-177.48	-178	10.01	0.58	2.00



Cert.No.: 24CH1379
Page.: 3 of 3

Calibration Results

Function : pH Measurement

Performing three buffers standard curve by using buffer nominal pH (4,7)(7,10)

Unit Under Calibration	Standard pH Buffer Solution	Actual pH Reading	Actual mV Reading (mV)	Uncertainty of pH Measurement (\pm)	Coverage factor k
pH Electrode S/N.:240710SIA605377	4.008	4.01	173	0.0079	2.00
	6.999	7.00	-2	0.0092	2.00
	6.999	7.00	-2	0.0095	2.00
	10.010	10.01	-178	0.0092	2.00

Function : Temperature Measurement

(*) Without adjustment

This equipment was connected with Temperature Probe;


- Model : -
- Serial No. : 240710SIA605377
Dimension of probe
- Length : 110 mm.
- Diameter : 12 mm.
- Immersion Depth : 100 mm.

Calibration Point (°C)	Standard Temperature (°C)	UUC* Reading (°C)	Error (°C)	Uncertainty of measurement (\pm °C)	Coverage factor k
15.0	15.003	14.9	-0.103	0.13	2.00
30.0	30.001	29.9	-0.101	0.13	2.00
45.0	45.003	44.8	-0.203	0.13	2.00

Remark : - UUC* = Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k, providing a level of confidence of approximately 95 %.

-000-



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLIANG, SUANLIANG BANGKOK 10250
TEL 0-2717-3000-29 FAX 0-2719-9484



Certificate of Calibration

Cert.No.: 24CH1070
Page.: 1 of 3

Equipment : pH Meter
Manufacturer : YSI
Model : pH100A
Serial No. : JC02729
ID No. : UAE.EFM.195/2561(ENV.pH.04/61)
Condition As-Received: Used Item
Received Date : 27 August 2024
Calibration Date : 28 August 2024
Reference : 2408-0882WSC-1
Submitted by : United Analyst and Engineering Consultant Co.,Ltd.
3 Soi Udomsuk 41, Sukhumvit Road,
Bangchak, Phrakhanong, Bangkok 10260

Ambient Temperature : (25 \pm 2.5) °C
Relative Humidity : (50 \pm 15) %
Calibration Procedure : In - house method :
- CP-CH5 by direct measurement with DC voltage standard and direct measurement with certified reference material (CRM)
- CP-CH8 by comparison with temperature standard

Calibrated by : Warakorn Lemaoatrakul

Approved by :
Approved Signatory

() Unnopphol Harachai
() Ponpan Paipim
(✓) Saithip Meangmai

Issue Date : 29 August 2024

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written Approval of the head of Corporate Services 3: Equipment Calibration and Testing Services.



Cert.No.: 24CH1070
Page.: 2 of 3

Condition of this calibration result

1. Reference Standard Instrument

Instrument	Serial No.	ID No.	Cert. No.	Due Date
1)Document Process Calibrator	43160066	130RC092	24E1320	22 Apr 2025
2)Ref. Standard Thermometer	2188080	130RC044	23I1216	10 Oct 2024

- This Certification is traceable to SI Through Technology Promotion Association (Thailand - Japan)

2. Certified Reference Materials :The measurement results are traceable to SI through Hach Lenge GmbH LT
Deutsche Akkreditierungsstelle, Accredited No.D-RM-15184-01-00

: The measurement results are traceable to SI through CPA chem Ltd.,
ANSI-ASQ National Accreditation Board, Accredited No. AR-1835

Buffer Solution	Manufacturer	Lot No.	Exp. date
pH 4.006	Hach Lenge GmbH	C03146	23 Feb 2026
pH 6.999	Hach Lenge GmbH	C03145	28 Feb 2026
pH 9.997	CPA chem	970853	25 Apr 2025

3. This certificate is valid only to the item calibrated on date and place of calibration.

Calibration Results

Function : mV Measurement

Performing standard curve by Document Process Calibrator at pH (4,7)(7,10)

Unit Under Calibration	Nominal Value	Standard Voltage Input	Actual Reading		Uncertainty of Measurement (\pm mV)	Coverage factor k
	pH	mV	mV	pH		
pH Meter S/N.: JC02729	4.00	177.48	177	4.01	0.58	2.00
	7.00	0.00	0	7.00	0.58	2.00
	7.00	0.00	0	7.00	0.58	2.00
	10.00	-177.48	-177	10.01	0.58	2.00



Cert.No.: 24CH1070
Page.: 3 of 3

Calibration Results

Function : pH Measurement

Performing three buffers standard curve by using buffer nominal pH (4,7)(7,10)

Unit Under Calibration	Standard pH Buffer Solution	Actual pH Reading	Actual mV Reading (mV)	Uncertainty of pH Measurement (±)	Coverage factor k
pH Electrode S/N: 231018SIA605377	4.006	4.01	173	0.0090	2.05
	6.999	7.00	-1	0.0084	2.00
	6.999	7.00	-1	0.0085	2.00
	9.997	10.00	-176	0.0092	2.00

Function : Temperature Measurement

(*) Without adjustment

This equipment was connected with Temperature Probe;

- Model : -
- Serial No. : 231018SIA605377
Dimension of probe
- Length : 110 mm.
- Diameter : 12 mm.
- Immersion Depth : 100 mm.

Calibration Point (°C)	Standard Temperature (°C)	UUC* Reading (°C)	Error (°C)	Uncertainty of measurement (± °C)	Coverage factor k
20.0	20.002	20.1	0.098	0.13	2.00
25.0	25.003	25.1	0.097	0.13	2.00
45.0	45.002	45.0	-0.002	0.13	2.00

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k, providing a level of confidence of approximately 95 %.

-o0o-

CERTIFICATE OF CALIBRATION

Certificate No. : SP24-018

Page 1 of 5

Customer : United Analyst and Engineering Consultant Co.,Ltd. (Head Office)

Address : 3 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260

Location of calibration : Laboratory 315

Equipment : UV-Vis Spectrophotometer

Manufacturer : Agilent Technologies

Model : Cary 60

Serial No. : MY15410009


ID No. : UAE.WAT.020/2558

Received Date : 7 May 2024

Calibration Date : 7 May 2024

Issue Date : 9 May 2024

Condition Instrument : Good

Calibrated by : 
(Mr.Tanawat Rittidach)

Technical Manager

Approved by : 
(Ms. Chonthicha Sangnern)

Quality Manager

The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only.

The measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the DQE Services Co., Ltd.

เอกสารไม่ควบคุม

REPORT OF CALIBRATION

Certificate No. : SP24-018

Page 2 of 5

Environment Condition : Ambient Temperature 25 ± 5 °C

Relative humidity 55 ± 20 %RH

Calibration method : In-house method CP-01 Based on ASTM E275-08

Certified Reference Materials :

Material	Serial No.	Certificate No.	Due date
Absorbance Standard set	25760	115663	25 October 2025
Absorbance Standard set	25757	115638	25 October 2025
Wavelength Standard set	25806	115657	25 October 2025
Wavelength Standard set	25758	115665	25 October 2025

Traceability : This certification is traceable to the International System of Unit maintained at National -

Institute of Standards and Technology (NIST) through Starna Scientific Limited

Spectral Band Width of UUC : 1.5 nm.

Scan Speed of UUC : 60 nm/min

Scan Interval of UUC : 0.15 nm.

Resolution of UUC : Photometric 0.0001 Abs.

Wavelength 0.1 nm.

เอกสารไม่ควบคุม

REPORT OF CALIBRATION

Certificate No. : SP24-018

Page 3 of 5



Calibration Results : Without adjustment

Photometric Accuracy :

Wavelength (nm.)	CRMs Values (Abs)	UUC Reading (Abs)	Correction (Abs)	Uncertainty (Abs)	Coverage factor k
420	0.0000	0.0000	0.0000	0.0028	2.00
	0.5780	0.5747	0.0033	0.0031	2.00
	1.0484	1.0438	0.0046	0.0029	2.00
	2.1876	2.1832	0.0044	0.0080	2.00
440	0.0000	0.0000	0.0000	0.0028	2.00
	0.5595	0.5581	0.0014	0.0034	2.00
	1.0239	1.0231	0.0008	0.0035	2.00
	2.1230	2.1219	0.0011	0.0080	2.00
465	0.0000	0.0000	0.0000	0.0028	2.00
	0.5230	0.5184	0.0046	0.0030	2.00
	0.9633	0.9614	0.0019	0.0029	2.00
	1.9753	1.9731	0.0022	0.0070	2.00
546.1	0.0000	0.0000	0.0000	0.0028	2.00
	0.5181	0.5150	0.0031	0.0031	2.00
	1.0002	0.9964	0.0038	0.0033	2.00
	1.9973	1.9914	0.0059	0.0088	2.00
590	0.0000	0.0000	0.0000	0.0028	2.00
	0.5517	0.5485	0.0032	0.0030	2.00
	1.0803	1.0772	0.0031	0.0030	2.00
	2.0373	2.0293	0.0080	0.0080	2.00
635	0.0000	0.0000	0.0000	0.0028	2.00
	0.5591	0.5565	0.0026	0.0031	2.00
	1.0518	1.0482	0.0036	0.0030	2.00
	1.9274	1.9202	0.0072	0.0079	2.00

เอกสารไม่ควบคุม

DQE Services Co.,Ltd.
32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Bangkok 10230
Phone : +66 (0)2 538 2054, Email : dqeservicesinfo@gmail.com





REPORT OF CALIBRATION

Certificate No. : SP24-018Page 4 of 5

Photometric Accuracy :

Wavelength (nm.)	CRMs Values (Abs)	UUC Reading (Abs)	Correction (Abs)	Uncertainty (Abs)	Coverage factor k
235	0.0000	0.0000	0.0000	0.0050	2.00
	0.7469	0.7435	0.0034	0.0057	2.00
257	0.0000	0.0000	0.0000	0.0050	2.00
	0.8674	0.8639	0.0035	0.0060	2.00
313	0.0000	0.0000	0.0000	0.0050	2.00
	0.2919	0.2907	0.0012	0.0051	2.00
350	0.0000	0.0000	0.0000	0.0050	2.00
	0.6430	0.6402	0.0028	0.0055	2.00

DQE Services Co.,Ltd.
32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Bangkok 10230
Phone : +66 (0)2 538 2054, Email : dqeservicesinfo@gmail.com



REPORT OF CALIBRATION

Certificate No. : SP24-018Page 5 of 5

Wavelength Accuracy :



CRMs Values (nm.)	UUC Reading (nm.)	Correction (nm.)	Uncertainty (nm.)	Coverage factor k
241.72	242.0	-0.28	0.18	2.00
279.45	279.5	-0.05	0.18	2.00
287.81	287.9	-0.09	0.18	2.00
334.06	333.9	0.16	0.18	2.00
360.93	360.5	0.43	0.18	2.00
418.59	418.1	0.49	0.18	2.00
445.94	445.6	0.34	0.18	2.00
453.66	453.3	0.36	0.18	2.00
460.02	459.8	0.22	0.18	2.00
536.59	536.0	0.59	0.18	2.00
637.98	638.7	-0.72	0.18	2.00
431.38	430.8	0.58	0.18	2.00
472.50	472.4	0.10	0.18	2.00
513.47	513.7	-0.23	0.18	2.00
528.88	529.1	-0.22	0.18	2.00
573.17	573.5	-0.33	0.18	2.00
585.35	585.2	0.15	0.20	2.00
684.40	685.1	-0.70	0.18	2.00
740.72	741.4	-0.68	0.20	2.00
748.55	749.1	-0.55	0.18	2.00
807.03	807.3	-0.27	0.18	2.00
879.28	879.3	-0.02	0.18	2.00

Remark : - UUC = Unit Under Calibration
- N/A = Not Available
- The result expanded uncertainty of measurement U is stated as the standard uncertainty of measurement multiplied by the coverage factor k, which for a normal distribution corresponds to a coverage probability of approximately 99%
- * Indicates non TISI accredited
- End of Certificate -

เอกสารไม่ควบคุม

เอกสารไม่ควบคุม

DQE Services Co.,Ltd.
32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Bangkok 10230
Phone : +66 (0)2 538 2054, Email : dqeservicesinfo@gmail.com



CERTIFICATE OF CALIBRATION

Certificate No. : SP25-019Page 1 of 5

Customer : United Analyst and Engineering Consultant Co.,Ltd. (Head Office)

Address : 3 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260

Location of calibration : Instrument room (207)

Equipment : UV-Vis Spectrophotometer

Manufacturer : Agilent Technologies

Model : Cary 60

Serial No. : MY15410009


ID No. : UAE.WAT.020/2558


Received Date : 26 May 2025

Calibration Date : 26 May 2025

Issue Date : 29 May 2025

Condition Instrument : Good

Calibrated by : 
(Mr.Tanawut Rittidach)
Technical Manager

Approved by : 
(Ms.Chonticha Sangnern)
Quality Manager



The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only.

The measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the DQE Services Co., Ltd.

เอกสารไม่ควบคุม

FM-708-02 R01 1/11/2021

DQE Services Co.,Ltd.
32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Bangkok 10230
Phone : +66 (0)2 538 2054, Email : dqeservicesinfo@gmail.com



REPORT OF CALIBRATION

Certificate No. : SP25-019Page 2 of 5

Environment Condition : Ambient Temperature 25 ± 5 °C
Relative humidity 55 ± 20 %RH

Calibration method : In-house method CP-01 Based on ASTM E275-08

Certified Reference Materials :

Material	Serial No.	Certificate No.	Due date
Absorbance Standard set	25760	115663	25 October 2025
Absorbance Standard set	25757	115638	25 October 2025
Wavelength Standard set	25806	115657	25 October 2025
Wavelength Standard set	25758	115665	25 October 2025

Traceability : This certification is traceable to the International System of Unit maintained at National -
Institute of Standards and Technology (NIST) through Starna Scientific Limited

Spectral Band Width of UUC : 1.5 nm.

Scan Speed of UUC : 60 nm/min



Scan Interval of UUC : 0.15 nm.

Resolution of UUC : Photometric 0.0001 Abs.
Wavelength 0.1 nm.

เอกสารไม่ควบคุม

FM-708-02 R01 1/11/2021

DQE Services Co.,Ltd.
32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Ladprao, Bangkok 10230
Phone : +66 (0)2 538 2054, Email : dqeservicesinfo@gmail.com



REPORT OF CALIBRATION

Certificate No. : SP25-019Page 3 of 5

Calibration Results : Without adjustment



Photometric Accuracy :

Wavelength (nm.)	CRMs Values (Abs)	UUC Reading (Abs)	Correction (Abs)	Uncertainty (Abs)	Coverage factor k
420	0.0000	0.0000	0.0000	0.0028	2.00
	0.5780	0.5739	0.0041	0.0031	2.00
	1.0484	1.0430	0.0054	0.0029	2.00
	2.1876	2.1876	0.0000	0.0084	2.00
440	0.0000	0.0000	0.0000	0.0028	2.00
	0.5595	0.5581	0.0014	0.0034	2.00
	1.0239	1.0219	0.0020	0.0035	2.00
	2.1230	2.1207	0.0023	0.0085	2.00
465	0.0000	0.0000	0.0000	0.0028	2.00
	0.5230	0.5190	0.0040	0.0029	2.00
	0.9633	0.9609	0.0024	0.0029	2.00
	1.9753	1.9719	0.0034	0.0079	2.00
546.1	0.0000	0.0000	0.0000	0.0028	2.00
	0.5181	0.5161	0.0020	0.0031	2.00
	1.0002	0.9979	0.0023	0.0033	2.00
	1.9973	2.0021	-0.0048	0.0102	2.00
590	0.0000	0.0000	0.0000	0.0028	2.00
	0.5517	0.5503	0.0014	0.0030	2.00
	1.0803	1.0808	-0.0005	0.0031	2.00
	2.0373	2.0324	0.0049	0.0105	2.00
635	0.0000	0.0000	0.0000	0.0028	2.00
	0.5591	0.5583	0.0008	0.0031	2.00
	1.0518	1.0513	0.0005	0.0030	2.00
	1.9274	1.9281	-0.0007	0.0102	2.00

เอกสารไม่ควบคุม

FM-708-02 R01 1/11/2021

DQE Services Co.,Ltd.
32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Ladprao, Bangkok 10230
Phone : +66 (0)2 538 2054, Email : dqeservicesinfo@gmail.com



REPORT OF CALIBRATION

Certificate No. : SP25-019Page 4 of 5



Photometric Accuracy :

Wavelength (nm.)	CRMs Values (Abs)	UUC Reading (Abs)	Correction (Abs)	Uncertainty (Abs)	Coverage factor k
235	0.0000	0.0000	0.0000	0.0050	2.00
	0.7469	0.7488	-0.0019	0.0063	2.00
257	0.0000	0.0000	0.0000	0.0050	2.00
	0.8674	0.8663	0.0011	0.0067	2.00
313	0.0000	0.0000	0.0000	0.0050	2.00
	0.2919	0.2902	0.0017	0.0052	2.00
350	0.0000	0.0000	0.0000	0.0050	2.00
	0.6430	0.6428	0.0002	0.0063	2.00

เอกสารไม่ควบคุม

FM-708-02 R01 1/11/2021

DQE Services Co.,Ltd.
32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Ladprao, Bangkok 10230
Phone : +66 (0)2 538 2054, Email : dqeservicesinfo@gmail.com



REPORT OF CALIBRATION

Certificate No. : SP25-019Page 5 of 5

Wavelength Accuracy :

CRMs Values (nm.)	UUC Reading (nm.)	Correction (nm.)	Uncertainty (nm.)	Coverage factor k
241.72	242.0	-0.28	0.18	2.00
279.45	279.5	-0.05	0.18	2.00
287.81	287.6	0.21	0.18	2.00
334.06	333.8	0.26	0.18	2.00
360.93	360.5	0.43	0.18	2.00
418.59	417.9	0.69	0.18	2.00
445.94	445.4	0.54	0.18	2.00
453.66	453.2	0.46	0.18	2.00
460.02	459.6	0.42	0.18	2.00
536.59	536.5	0.09	0.18	2.00
637.98	638.5	-0.52	0.18	2.00
431.38	430.7	0.68	0.18	2.00
472.50	472.3	0.20	0.18	2.00
513.47	513.5	-0.03	0.18	2.00
528.88	528.9	-0.02	0.18	2.00
573.17	573.8	-0.63	0.18	2.00
585.35	585.2	0.15	0.20	2.00
684.40	685.1	-0.70	0.18	2.00
740.72	741.1	-0.38	0.20	2.00
748.55	748.9	-0.35	0.18	2.00
807.03	807.1	-0.07	0.18	2.00
879.28	879.1	0.18	0.18	2.00


Remark : - UUC = Unit Under Calibration
- N/A = Not Available
- The result expanded uncertainty of measurement U is stated as the standard uncertainty of measurement multiplied by the coverage factor k,
which for a normal distribution corresponds to a coverage probability of approximately 95%

- End of Certificate -

เอกสารไม่ควบคุม

FM-708-02 R01 1/11/2021

DQE Services Co.,Ltd.
32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Ladprao, Bangkok 10230
Phone : +66 (0)2 538 2054, Email : dqeservicesinfo@gmail.com



CERTIFICATE OF CALIBRATION

Certificate No. : SP24-008Page 1 of 5

Customer : United Analyst and Engineering Consultant Co.,Ltd. (Head Office)

Address : 3 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260

Location of calibration : Laboratory 315

Equipment : UV-Vis Spectrophotometer

Manufacturer : Hitachi

Model : U-1900

Serial No. : 2021-064

ID No. : UAE.WAS.006/2552


Received Date : 16 January 2024

Calibration Date : 16 January 2024

Issue Date : 19 January 2024

Condition Instrument : Good

Calibrated by : 
(Mr.Tanawat Rittidach)
Technical Manager

Approved by : 
(Ms. Chonthicha Sangnern)
Quality Manager

The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only.

The measurement capability of the laboratory and its conformity to recognized national standards used to the units of measurement realized as the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the DQE Services Co., Ltd.

เอกสารไม่ควบคุม

FM-708-02 R01 1/11/2021

REPORT OF CALIBRATION

Certificate No. : SP24-008

Page 2 of 5

Environment Condition : Ambient Temperature 25 ± 5 °CRelative humidity 55 ± 20 %RH

Calibration method : In-house method CP-01 Based on ASTM E275-08

Certified Reference Materials :

Material	Serial No.	Certificate No.	Due date
Absorbance Standard set	25760	115663	25 October 2025
Absorbance Standard set	25757	115638	25 October 2025
Wavelength Standard set	25806	115657	25 October 2025
Wavelength Standard set	25758	115665	25 October 2025

Traceability : This certification is traceable to the International System of Unit maintained at National -

Institute of Standards and Technology (NIST) through Starna Scientific Limited

Spectral Band Width of UUC : 4.0 nm.

Scan Speed of UUC : 200 nm/min

Scan Interval of UUC : 0.1 nm.

Resolution of UUC : Photometric 0.001 Abs.

Wavelength 0.1 nm.

เอกสารไม่ควบคุม

FM-708-02 R01 1/11/2021

REPORT OF CALIBRATION

Certificate No. : SP24-008

Page 3 of 5

Calibration Results : Without adjustment

Photometric Accuracy :

Wavelength (nm.)	CRMs Values (Abs)	UUC Reading (Abs)	Correction (Abs)	Uncertainty (Abs)	Coverage factor k
420	0.0000	0.000	0.0000	0.0028	2.00
	0.5780	0.575	0.0030	0.0031	2.00
	1.0484	1.046	0.0024	0.0029	2.00
	2.1876	2.186	0.0016	0.0080	2.00
440	0.0000	0.000	0.0000	0.0028	2.00
	0.5595	0.558	0.0015	0.0034	2.00
	1.0239	1.024	-0.0001	0.0035	2.00
	2.1230	2.121	0.0020	0.0079	2.00
465	0.0000	0.000	0.0000	0.0028	2.00
	0.5230	0.520	0.0030	0.0030	2.00
	0.9633	0.961	0.0023	0.0029	2.00
	1.9753	1.975	0.0003	0.0070	2.00
546.1	0.0000	0.000	0.0000	0.0028	2.00
	0.5181	0.516	0.0021	0.0031	2.00
	1.0002	0.999	0.0012	0.0033	2.00
	1.9973	1.994	0.0033	0.0084	2.00
590	0.0000	0.000	0.0000	0.0028	2.00
	0.5517	0.550	0.0017	0.0030	2.00
	1.0803	1.080	0.0003	0.0030	2.00
	2.0373	2.032	0.0053	0.0080	2.00
635	0.0000	0.000	0.0000	0.0028	2.00
	0.5591	0.558	0.0011	0.0031	2.00
	1.0518	1.051	0.0008	0.0030	2.00
	1.9274	1.923	0.0044	0.0079	2.00

เอกสารไม่ควบคุม

FM-708-02 R01 1/11/2021

REPORT OF CALIBRATION

Certificate No. : SP24-008

Page 4 of 5

Photometric Accuracy :

Wavelength (nm.)	CRMs Values (Abs)	UUC Reading (Abs)	Correction (Abs)	Uncertainty (Abs)	Coverage factor k
235	0.0000	0.000	0.0000	0.0050	2.00
	0.7469	0.748	-0.0011	0.0057	2.00
257	0.0000	0.000	0.0000	0.0050	2.00
	0.8674	0.865	0.0024	0.0059	2.00
313	0.0000	0.000	0.0000	0.0050	2.00
	0.2919	0.293	-0.0011	0.0051	2.00
350	0.0000	0.000	0.0000	0.0050	2.00
	0.6430	0.641	0.0020	0.0055	2.00

เอกสารไม่ควบคุม

FM-708-02 R01 1/11/2021

REPORT OF CALIBRATION

Certificate No. : SP24-008

Page 5 of 5

Wavelength Accuracy :

CRMs Values (nm.)	UUC Reading (nm.)	Correction (nm.)	Uncertainty (nm.)	Coverage factor k
241.54	241.1	0.44	0.18	2.00
279.40	278.9	0.50	0.18	2.00
288.70	288.0	0.70	0.18	2.00
334.22	333.8	0.42	0.18	2.00
361.26	360.8	0.46	0.18	2.00
418.48	418.2	0.28	0.18	2.00
446.70	446.0	0.70	0.18	2.00
453.20	453.1	0.10	0.18	2.00
460.06	459.6	0.46	0.18	2.00
536.90	536.4	0.50	0.18	2.00
637.94	637.6	0.34	0.18	2.00
440.74	440.1	0.64	0.18	2.00
472.22	472.0	0.22	0.18	2.00
513.70	513.5	0.20	0.18	2.00
528.72	528.2	0.52	0.18	2.00
574.60	574.3	0.30	0.18	2.00
585.48	585.0	0.48	0.20	2.00
684.63	684.2	0.43	0.18	2.00
740.27	740.0	0.27	0.20	2.00
748.28	747.8	0.48	0.18	2.00
807.16	806.8	0.36	0.18	2.00
879.70	879.2	0.50	0.18	2.00

Remark : - UUC = Unit Under Calibration

- N/A = Not Available

- The result expanded uncertainty of measurement U is stated as the standard uncertainty of measurement multiplied by the coverage factor k,

which for a normal distribution corresponds to a coverage probability of approximately 95%


- * Indicates non TISI accredited

- End of Certificate -

เอกสารไม่ควบคุม

FM-708-02 R01 1/11/2021

DQE Services Co.,Ltd.
32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Bangkok 10230
Phone : +66 (0)2 538 2054, Email : dqeservicesinfo@gmail.com


ISO 9001:2015
CALIBRATION DATA

CERTIFICATE OF CALIBRATION

Certificate No. : SP25-001Page 1 of 5

Customer : United Analyst and Engineering Consultant Co.,Ltd. (Head Office)

Address : 3 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260

Location of calibration : Laboratory 213

Equipment : UV-Vis Spectrophotometer

Manufacturer : Hitachi

Model : U-2900

Serial No. : 21E22-009

ID No. : UAE.WAT.051/2564

Received Date : 3 January 2025

Calibration Date : 3 January 2025

Issue Date : 8 January 2025

Condition Instrument : Good

Calibrated by : (Mr.Tanawat Rittidach)Approved by : (Ms.Chonthicha Sangnern)

Technical Manager

Quality Manager

The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only.

The measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written consent of DQE Services Co., Ltd.

เอกสารไม่ควบคุม

FM-708-02 R01 1/11/2021

DQE Services Co.,Ltd.
32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Bangkok 10230
Phone : +66 (0)2 538 2054, Email : dqeservicesinfo@gmail.com


ISO 9001:2015
CALIBRATION DATA

REPORT OF CALIBRATION

Certificate No. : SP25-001Page 2 of 5

Environment Condition : Ambient Temperature 25 ± 5 °C

Relative humidity 55 ± 20 %RH

Calibration method : In-house method CP-01 Based on ASTM E275-08

Certified Reference Materials :

Material	Serial No.	Certificate No.	Due date
Absorbance Standard set	25760	115663	25 October 2025
Absorbance Standard set	25757	115638	25 October 2025
Wavelength Standard set	25806	115657	25 October 2025
Wavelength Standard set	25758	115665	25 October 2025

Traceability : This certification is traceable to the International System of Unit maintained at National -
Institute of Standards and Technology (NIST) through Starna Scientific Limited

Spectral Band Width of UUC : 1.5 nm.

Scan Speed of UUC : 200 nm/min

Scan Interval of UUC : 0.1 nm.


Resolution of UUC : Photometric 0.001 Abs.

Wavelength 0.1 nm.

เอกสารไม่ควบคุม

FM-708-02 R01 1/11/2021

DQE Services Co.,Ltd.
32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Bangkok 10230
Phone : +66 (0)2 538 2054, Email : dqeservicesinfo@gmail.com


ISO 9001:2015
CALIBRATION DATA

REPORT OF CALIBRATION

Certificate No. : SP25-001Page 3 of 5

Calibration Results : Without adjustment


Photometric Accuracy :

Wavelength (nm.)	CRMs Values (Abs)	UUC Reading (Abs)	Correction (Abs)	Uncertainty (Abs)	Coverage factor k
420	0.0000	0.000	0.0000	0.0028	2.00
	0.5780	0.578	0.0000	0.0031	2.00
	1.0484	1.045	0.0034	0.0029	2.00
	2.1876	2.192	-0.0044	0.0075	2.00
440	0.0000	0.000	0.0000	0.0028	2.00
	0.5595	0.560	-0.0005	0.0034	2.00
	1.0239	1.023	0.0009	0.0035	2.00
	2.1230	2.125	-0.0020	0.0079	2.00
465	0.0000	0.000	0.0000	0.0028	2.00
	0.5230	0.521	0.0020	0.0030	2.00
	0.9633	0.961	0.0023	0.0029	2.00
	1.9753	1.977	-0.0017	0.0070	2.00
546.1	0.0000	0.000	0.0000	0.0028	2.00
	0.5181	0.518	0.0001	0.0031	2.00
	1.0002	0.998	0.0022	0.0033	2.00
	1.9973	1.993	0.0043	0.0084	2.00
590	0.0000	0.000	0.0000	0.0028	2.00
	0.5517	0.552	-0.0003	0.0030	2.00
	1.0803	1.079	0.0013	0.0030	2.00
	2.0373	2.032	0.0053	0.0079	2.00
635	0.0000	0.000	0.0000	0.0028	2.00
	0.5591	0.559	0.0001	0.0031	2.00
	1.0518	1.050	0.0018	0.0030	2.00
	1.9274	1.923	0.0044	0.0079	2.00

เอกสารไม่ควบคุม

FM-708-02 R01 1/11/2021

DQE Services Co.,Ltd.
32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Bangkok 10230
Phone : +66 (0)2 538 2054, Email : dqeservicesinfo@gmail.com


ISO 9001:2015
CALIBRATION DATA

REPORT OF CALIBRATION

Certificate No. : SP25-001Page 4 of 5



Photometric Accuracy :

Wavelength (nm.)	CRMs Values (Abs)	UUC Reading (Abs)	Correction (Abs)	Uncertainty (Abs)	Coverage factor k
235	0.0000	0.000	0.0000	0.0050	2.00
	0.7469	0.744	0.0029	0.0057	2.00
257	0.0000	0.000	0.0000	0.0050	2.00
	0.8674	0.863	0.0044	0.0059	2.00
313	0.0000	0.000	0.0000	0.0050	2.00
	0.2919	0.290	0.0019	0.0051	2.00
350	0.0000	0.000	0.0000	0.0050	2.00
	0.6430	0.640	0.0030	0.0055	2.00

เอกสารไม่ควบคุม

FM-708-02 R01 1/11/2021

DQE Services Co.,Ltd.
32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Bangkok 10230
Phone : +66 (0)2 538 2054, Email : dqeservicesinfo@gmail.com



REPORT OF CALIBRATION

Certificate No. : SP25-001Page 5 of 5

Wavelength Accuracy :



CRMs Values (nm.)	UUC Reading (nm.)	Correction (nm.)	Uncertainty (nm.)	Coverage factor k
241.72	241.1	0.62	0.18	2.00
279.45	279.0	0.45	0.18	2.00
287.81	287.3	0.51	0.18	2.00
334.06	333.8	0.26	0.18	2.00
360.93	360.6	0.33	0.18	2.00
418.59	418.2	0.39	0.18	2.00
445.94	445.5	0.44	0.18	2.00
453.66	453.4	0.26	0.18	2.00
460.02	459.8	0.22	0.18	2.00
536.59	536.6	-0.01	0.18	2.00
637.98	637.7	0.28	0.18	2.00
431.38	431.1	0.28	0.18	2.00
472.50	472.3	0.20	0.18	2.00
513.47	513.4	0.07	0.18	2.00
528.88	528.9	-0.02	0.18	2.00
573.17	573.3	-0.13	0.18	2.00
585.35	585.1	0.25	0.20	2.00
684.40	684.5	-0.10	0.18	2.00
740.72	741.0	-0.28	0.20	2.00
748.55	748.8	-0.25	0.18	2.00
807.03	807.3	-0.27	0.18	2.00
879.28	879.6	-0.32	0.18	2.00

Remark : - UUC = Unit Under Calibration
- N/A = Not Available
- The result expanded uncertainty of measurement U is stated as the standard uncertainty of measurement multiplied by the coverage factor k ,
which for a normal distribution corresponds to a coverage probability of approximately 95%
- End of Certificate -

เอกสารไม่ควบคุม

FM-708-02 R01 1/11/2021

DQE Services Co.,Ltd.
32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Bangkok 10230
Phone : +66 (0)2 538 2054, Email : dqeservicesinfo@gmail.com



CERTIFICATE OF CALIBRATION

Certificate No. : SP24-028Page 1 of 5

Customer : United Analyst and Engineering Consultant Co.,Ltd. (Head Office)

Address : 3 Soi Udumsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260

Location of calibration : Laboratory 315

Equipment : UV-Vis Spectrophotometer

Manufacturer : HITACHI

Model : U-5100

Serial No. : 23A4-008


ID No. : UAE.WAS.010/2567


Received Date : 10 September 2024

Calibration Date : 10 September 2024

Issue Date : 13 September 2024

Condition Instrument : Good

Calibrated by : 
(Mr.Tanawut Rittidach)
Technical Manager

Approved by : 
(Ms. Chonthicha Sangngern)
Quality Manager



The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only.

The measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the DQE Services Co., Ltd.

เอกสารไม่ควบคุม

FM-708-02 R01 1/11/2021

DQE Services Co.,Ltd.
32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Bangkok 10230
Phone : +66 (0)2 538 2054, Email : dqeservicesinfo@gmail.com



REPORT OF CALIBRATION

Certificate No. : SP24-028Page 2 of 5

Environment Condition : Ambient Temperature 25 ± 5 °C
Relative humidity 55 ± 20 %RH

Calibration method : In-house method CP-01 Based on ASTM E275-08

Certified Reference Materials :

Material	Serial No.	Certificate No.	Due date
Absorbance Standard set	25760	115663	25 October 2025
Absorbance Standard set	25757	115638	25 October 2025
Wavelength Standard set	25806	115657	25 October 2025
Wavelength Standard set	25758	115665	25 October 2025

Traceability : This certification is traceable to the International System of Unit maintained at National -
Institute of Standards and Technology (NIST) through Sarna Scientific Limited

Spectral Band Width of UUC : 5.0 nm.

Scan Speed of UUC : 40



Scan Interval of UUC : 0.1 nm.

Resolution of UUC : Photometric 0.001 Abs.
Wavelength 0.1 nm.

เอกสารไม่ควบคุม

FM-708-02 R01 1/11/2021

DQE Services Co.,Ltd.
32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Bangkok 10230
Phone : +66 (0)2 538 2054, Email : dqeservicesinfo@gmail.com



REPORT OF CALIBRATION

Certificate No. : SP24-028Page 3 of 5

Calibration Results : Without adjustment

Photometric Accuracy :

Wavelength (nm.)	CRMs Values (Abs)	UUC Reading (Abs)	Correction (Abs)	Uncertainty (Abs)	Coverage factor k
420	0.0000	0.000	0.0000	0.0028	2.00
	0.5780	0.575	0.0030	0.0031	2.00
	1.0484	1.044	0.0044	0.0029	2.00
	2.1876	2.190	-0.0024	0.0075	2.00
440	0.0000	0.000	0.0000	0.0028	2.00
	0.5595	0.557	0.0025	0.0034	2.00
	1.0239	1.021	0.0029	0.0035	2.00
	2.1230	2.121	0.0020	0.0079	2.00
465	0.0000	0.000	0.0000	0.0028	2.00
	0.5230	0.519	0.0040	0.0029	2.00
	0.9633	0.961	0.0023	0.0028	2.00
	1.9753	1.975	0.0003	0.0070	2.00
546.1	0.0000	0.000	0.0000	0.0028	2.00
	0.5181	0.515	0.0031	0.0031	2.00
	1.0002	0.997	0.0032	0.0033	2.00
	1.9973	1.996	0.0013	0.0085	2.00
590	0.0000	0.000	0.0000	0.0028	2.00
	0.5517	0.549	0.0027	0.0030	2.00
	1.0803	1.078	0.0023	0.0029	2.00
	2.0373	2.031	0.0063	0.0081	2.00
635	0.0000	0.000	0.0000	0.0028	2.00
	0.5591	0.557	0.0021	0.0031	2.00
	1.0518	1.049	0.0028	0.0029	2.00
	1.9274	1.923	0.0044	0.0080	2.00

เอกสารไม่ควบคุม

FM-708-02 R01 1/11/2021

REPORT OF CALIBRATION

Certificate No. : SP24-028

Page 4 of 5

Photometric Accuracy :

Wavelength (nm.)	CRMs Values (Abs)	UUC Reading (Abs)	Correction (Abs)	Uncertainty (Abs)	Coverage factor k
235	0.0000	0.000	0.0000	0.0050	2.00
	0.7469	0.743	0.0039	0.0056	2.00
257	0.0000	0.000	0.0000	0.0050	2.00
	0.8674	0.862	0.0054	0.0059	2.00
313	0.0000	0.000	0.0000	0.0050	2.00
	0.2919	0.291	0.0009	0.0051	2.00
350	0.0000	0.000	0.0000	0.0050	2.00
	0.6430	0.639	0.0040	0.0055	2.00

REPORT OF CALIBRATION

Certificate No. : SP24-028

Page 5 of 5

Wavelength Accuracy :

CRMs Values (nm.)	UUC Reading (nm.)	Correction (nm.)	Uncertainty (nm.)	Coverage factor k
241.00	240.4	0.60	0.18	2.00
279.30	278.7	0.60	0.18	2.00
288.90	288.5	0.40	0.18	2.00
334.50	334.2	0.30	0.18	2.00
361.40	361.1	0.30	0.18	2.00
418.40	418.0	0.40	0.18	2.00
447.20	446.7	0.50	0.18	2.00
459.30	459.6	-0.30	0.18	2.00
537.00	536.6	0.40	0.18	2.00
638.00	637.4	0.60	0.18	2.00
441.29	440.8	0.49	0.18	2.00
479.88	479.6	0.28	0.18	2.00
513.75	513.5	0.25	0.18	2.00
528.59	528.6	-0.01	0.18	2.00
575.10	574.9	0.20	0.18	2.00
585.56	585.3	0.26	0.20	2.00
684.70	684.1	0.60	0.18	2.00
740.51	740.0	0.51	0.20	2.00
747.61	747.2	0.41	0.18	2.00
807.04	806.3	0.74	0.18	2.00
879.68	878.9	0.78	0.18	2.00

Remark : - UUC = Unit Under Calibration

- N/A = Not Available

- The result expanded uncertainty of measurement U is stated as the standard uncertainty of measurement multiplied by the coverage factor k.

which for a normal distribution corresponds to a coverage probability of approximately 95%

- End of Certificate -

เอกสารไม่ควบคุม

FM-708-02 R01 1/11/2021

เอกสารไม่ควบคุม

FM-708-02 R01 1/11/2021

Calibration Certificate

Certificate No.: 2502228-003-01
Client name: UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.
Address: 3 Soi Udomsuk 41, Sukhumvit Road,
Bangchack, Prakhnong, Bangkok 10260

Page 1 of 3

Equipment: Electronic Balance
Manufacturer: METTLER TOLEDO
Model: MS204TS/00
Serial No.: C252436235
ID No.: UAE.AIR.023/2566
Order No.: 2502228
Operation No.: 2502228-003
Date of Receipt: 19 March 2025
Date of Calibration: 19 March 2025

Calibrated by Mr.Yothin Charoensuk **Approved by** *N. Niyadatt*
Scientist (Mr.Pheraphat Tuanjit)
Manager, Division of Calibration Laboratory
Responsible for the Technical Management Team
Date of Issue: 25 March 2025

The uncertainties are for a confidence probability of approximately 95%

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the National Food Institute.

FCS-009 Revision: 01 Date: 20-04-65

เอกสารไม่ควบคุม เอกสารไม่ควบคุม
2008 Soi 35, Anur Adorn Road, Bang Yi Khan Subdistrict, Bang Phai District, Bangkok 10710, Thailand
Tel: +66(0) 2422 8568 Fax: +66(0) 2422 8545 nfi.com

Calibration Report

Certificate No.: 2502228-003-01
Equipment: Electronic Balance
Manufacturer: METTLER TOLEDO
Model: MS204TS/00
Resolution: 0.0001 g
Serial No.: C252436235
ID No.: UAE.AIR.023/2566
Capacity: 220 g

Page 2 of 3

Date of Calibration: 19 March 2025
Environment Condition: Ambient Temperature: 21.1 ± 0.6 °C Relative Humidity: 55 ± 0.75 %
Place of Calibration: 206 Balance Room 2, UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.
Condition of Equipment: Good Condition
Condition of This Results of Calibration:
1. Calibration Method: NFI Method W-MA-001 In-House Method based on UKAS Lab 14 : 2019
2. Reference Standards:
Reference Standard **Model** **Serial No.** **Calibrated By** **Certificate No.** **Due Date**
Standard Weight Class E2 1mg to 200g 8505567572 TCS M24041005 19 April 2025
Instrument **Model** **Serial No.** **Calibrated By** **Certificate No.** **Due Date**
Thermo-Hygro Meter 608-H1 NFI.BTH 017/23 Quality Reborn QR25-0542 10 February 2025
3. This certification is traceable to SI UNIT
4. This certificate was certified only for the instrument we calibrated.
5. This result of calibration was found accurate as shown on date and place of calibration only.

Calibration Results:

1. Repeatability of Reading:

Nominal Value (g)	Standard Deviation of Reading (g)
100	0.000052
200	0.000079

2. Off-Center Error:

A mass of 200 g was placed and moved to various position on pan.

The balance reading obtained is given in the table.

1	2	3
4	5	6
(g)	(g)	(g)
99.9997	99.9995	99.9995
99.9997	99.9997	99.9999
99.9999	99.9998	0.0003

FCS-012 Revision: 01 Date: 20-04-65

เอกสารไม่ควบคุม เอกสารไม่ควบคุม
2008 Soi 35, Anur Adorn Road, Bang Yi Khan Subdistrict, Bang Phai District, Bangkok 10710, Thailand
Tel: +66(0) 2422 8568 Fax: +66(0) 2422 8545 nfi.com

Calibration Report

Certificate No.: 2502228-003-01
Equipment: Electronic Balance
Manufacturer: METTLER TOLEDO
Model: MS204TS/00
Resolution: 0.0001 g
Serial No.: C252436235
ID No.: UAE.AIR.023/2566
Capacity: 220 g

Page 3 of 3

Date of Calibration: 19 March 2025
Calibration Results: (Continued)
Calibration Range: 0-200 g
Calibration Adjustment: Internal Calibration
3. Departure from Nominal Value:

Nominal Value (g)	Standard Value (g)	Average Reading (g)	Correction (g)	Uncertainty (± g)	Coverage Factor k
Unload	0.00000	0.0000	0.0000	0.000089	2.00
0.1	0.10001	0.1001	-0.0001	0.000089	2.00
1	1.00000	1.0000	0.0000	0.000089	2.00
3	3.00003	3.0000	0.0000	0.000091	2.00
5	5.00002	5.0000	0.0000	0.000090	2.00
10	10.00001	9.9999	0.0001	0.000092	2.00
20	20.00003	20.0000	0.0000	0.000096	2.00
50	50.00003	49.9998	0.0002	0.00012	2.00
70	70.00006	69.9998	0.0003	0.00013	2.00
100	100.00006	99.9998	0.0003	0.00016	2.00
150	150.00009	150.0000	0.0001	0.00021	2.00
200	200.00013	200.0000	0.0001	0.00029	2.00

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k, providing a level of confidence of approximately 95 %.

----- End -----

FCS-012 Revision: 01 Date: 20-04-65

เอกสารไม่ควบคุม เอกสารไม่ควบคุม
2008 Soi 35, Anur Adorn Road, Bang Yi Khan Subdistrict, Bang Phai District, Bangkok 10710, Thailand
Tel: +66(0) 2422 8568 Fax: +66(0) 2422 8545 nfi.com

List of Instruments Certification for Air & Noise Quality Analysis

No.	Instrument/Equipment	Parameter	Manufacturer	Model/Serial No.	Calibrator	Certification No.	Date of Calibration	Due date of Calibration	Remark
Ambient									
1	Orifice Transfer Standard Calibrator	Total Suspended Particulate (TSP)	Tisch Environmental, Inc.	TE-5025A 3383	Jiranatee Associates Co., Ltd.	COF-039-67	27 Sep 24	26 Sep 25	-
2	U-Tube Manometer	Total Suspended Particulate (TSP)	Dwyer	121-36-W/M -	Technology Promotion Association (Thailand-Japan)	25P112	19 Feb 25	18 Feb 26	-
3	Aneroid Barometer	Total Suspended Particulate (TSP)	Barigo, Germany	-	Technology Promotion Association (Thailand-Japan)	24P1856	4 Jun 24	3 Jun 25	-
4	Digital Thermo - Hygrometer	Total Suspended Particulate (TSP)	Digicon	TH-02 435031148	Technology Promotion Association (Thailand-Japan)	24H1487	15 Jul 24	14 Jul 25	-
5	Nitrogen Dioxide Analyzer	Nitrogen Dioxide	Thermo Scientific	42i CM19050148	UAE Consultant Co., Ltd.	20092024	20 Sep 24	19 Sep 25	-
6	Nitrogen Dioxide Analyzer	Nitrogen Dioxide	Thermo Scientific	42i CM19050149	UAE Consultant Co., Ltd.	17092024	17 Sep 24	16 Sep 25	-
7	Nitrogen Dioxide Analyzer	Nitrogen Dioxide	Thermo Scientific	42i 1201778105	UAE Consultant Co., Ltd.	26092024	26 Sep 24	25 Sep 25	-
8	Nitrogen Dioxide Analyzer	Nitrogen Dioxide	Thermo Scientific	42i 1201778106	UAE Consultant Co., Ltd.	20092024	20 Sep 24	19 Sep 25	-
9	Standard Gases (Mixture)	Nitrogen Dioxide	Airgas	EB0162121 2016PSIG	Airgas an Air Liquide company	E05NI91E15A0014	6 Jun 23	6 Jun 31	-
10	Sulphur Dioxide Analyzer	Sulphur Dioxide	Thermo Scientific	43i CM22387061	UAE Consultant Co., Ltd.	06092024	6 Sep 24	5 Sep 25	-
11	Sulphur Dioxide Analyzer	Sulphur Dioxide	Thermo Scientific	43i CM22387063	UAE Consultant Co., Ltd.	19062024	19 Jun 24	18 Jun 25	-
12	Sulphur Dioxide Analyzer	Sulphur Dioxide	Thermo Scientific	43i 1201778113	UAE Consultant Co., Ltd.	04092024	4 Sep 24	3 Sep 25	-
13	Sulphur Dioxide Analyzer	Sulphur Dioxide	Thermo Scientific	43i 1201778116	UAE Consultant Co., Ltd.	19062024	19 Jun 24	18 Jun 25	-
14	Standard Gases (Mixture)	Sulphur Dioxide	Airgas	EB0162121 2016PSIG	Airgas an Air Liquide company	E05NI91E15A0014	6 Jun 23	6 Jun 31	-

List of Instruments Certification for Air & Noise Quality Analysis

No.	Instrument/Equipment	Parameter	Manufacturer	Model/Serial No.	Calibrator	Certification No.	Date of Calibration	Due date of Calibration	Remark
Ambient									
15	Wind Speed/Wind Direction	WS/WD	Scarlet Tech Ltd.	WL-21 2111DR0072	Thai Meteorological Department	001/25	3 Jan 25	2 Jan 26	-
16	Wind Speed/Wind Direction	WS/WD	Scarlet Tech Ltd.	WL-21 2205DR0113	Thai Meteorological Department	002/25	3 Jan 25	2 Jan 26	-
17	Wind Speed/Wind Direction	WS/WD	LSI Lastem	DNA202/E-LOG BQ1705627/17037708	Jiranatee Associates Co., Ltd.	CWS-027-67	7 Aug 24	6 Aug 25	-
18	Wind Speed/Wind Direction	WS/WD	LSI Lastem	DNA202/E-LOG BQ1705626/17037713	Jiranatee Associates Co., Ltd.	CWS-028-67	7 Aug 24	6 Aug 25	-
19	Sound Level Calibrator (Acoustic Calibrator)	Calibrate Sound Level Meter	01dB	CAL31 84065	Innovative Instrument Co.,Ltd.	24-ACT-087	25 Jun 24	24 Jun 25	-
20	Sound Level Meter	L _{Aeq} 24 hrs	Larson Davis	LxT2 0005299	Innovative Instrument Co.,Ltd.	24-SLM-240	11 Jul 24	10 Jul 25	-
21	Sound Level Meter	L _{Aeq} 24 hrs	Larson Davis	LxT2 0005372	Innovative Instrument Co.,Ltd.	24-SLM-229	9 Jul 24	8 Jul 25	-
22	Sound Level Meter	L _{Aeq} 24 hrs	Larson Davis	LxT2 0005286	Innovative Instrument Co.,Ltd.	24-SLM-234	10 Jul 24	9 Jul 25	-
23	Sound Level Meter	L _{Aeq} 24 hrs	Larson Davis	LxT2 0005290	Innovative Instrument Co.,Ltd.	24-SLM-238	11 Jul 24	10 Jul 25	-
24	Sound Level Meter	L _{Aeq} 24 hrs	Larson Davis	LxT2 0005293	Innovative Instrument Co.,Ltd.	24-SLM-231	10 Jul 24	9 Jul 25	-
25	Sound Level Meter	L _{Aeq} 24 hrs	Larson Davis	LxT2 0005341	Innovative Instrument Co.,Ltd.	24-SLM-232	10 Jul 24	9 Jul 25	-
26	Sound Level Meter	L _{Aeq} 24 hrs	Larson Davis	LxT2 0005346	Innovative Instrument Co.,Ltd.	24-SLM-235	10 Jul 24	9 Jul 25	-
27	Sound Level Meter	L _{Aeq} 24 hrs	Larson Davis	LxT2 0005348	Electrical And Electronics Institute Foundation For Industrial Development	CP20240292EA	6 Aug 24	5 Aug 25	-

List of Instruments Certification for Water Quality Analysis

No.	Instrument/Equipment	Parameter	Manufacturer	Model/Serial No.	Calibrator	Certification No.	Date of Calibration	Due date of Calibration	Remark
Water									
1	pH Meter	pH	Horiba	LAQUA-PH210 HA1G0008	Technology Promotion Association (Thailand-Japan)	24CH1153/1	18 Sep 24	17 Sep 25	-
2	DO Meter	DO	Horiba	LAQUA-DO210 HE1D0010	Technology Promotion Association (Thailand-Japan)	24TW200	18 Sep 24	17 Sep 25	-

CERTIFICATE OF CALIBRATION

Certificate No. : COF-039-67

Page 1 of 2 Pages

MEASUREMENT ITEM
MANUFACTURER : Top Load Orifice
MODEL/TYPE : TSC1
SERIAL NUMBER : TE-S025A
ID NUMBER : 3383
CONDITION AS-RECEIVED : UAE EFM 063/2560
CUSTOMER : Used Item
United Analyst and Engineering Consultant Co., Ltd.
81 Soi Udomsuk 41, Sukhumvit Road, Bangkok, Phrakhanong,
Bangkok 10260

RECEIVED DATE : 16 Sep 2024
MEASUREMENT DATE : 27 Sep 2024
ISSUE DATE : 27 Sep 2024

ENVIRONMENTAL CONDITIONS:

Ambient condition in the laboratory are as follow:

Temperature : 23.0 ± 3.0 °C
Relative Humidity : 55.0 ± 15.0 %RH
Atmospheric Pressure : 1020 ± 10 hPa

CALIBRATION CONDITION:

Preconditioning : 24 hours at ambient conditions.
Measurement Condition : The average values during measurement are 23.9 °C and 45.0 %RH.

NOTED: The certificate is valid only to the item calibrated on date and place of calibration

TABULATION OF RESULTS:

The table on next page give the measured values.

Calibrated by:
☐ Mr. Sorawat Thachulad
☒ Miss Jiraporn Lertsomphol



Approved signature:
Mr. Parinya Booncharoen
Calibration Department Manager

MEASUREMENT RESULTS:

The Orifice gas flow device was calibrated by direct comparison method with the Standard Rotary Displacement Meter (Roots Meter). The humid air was used as a medium in the system. The standard conditions are 25 °C (298.15 K) and 760 mmHg for standard temperature and standard pressure respectively.

Table 1: The results of Q Standard calibration data

Plate	Flow rate m^3/min	Pressure [Pa] mmHg	Temperature [Ta] °C	Temperature [Tm] °C	Ap_meter mmHg	Ap_Orifice mmHg	Y	Standard Flow [Qs] m^3/min
1	0.703	758.131	23.02	22.49	56.556	1.738	1.319	0.654
2	1.000	758.205	23.70	22.83	63.034	3.473	1.965	0.922
3	1.121	758.284	23.64	22.69	42.633	4.642	2.157	1.064
4	1.367	758.274	23.64	22.65	31.359	5.197	2.282	1.125
5	1.409	758.325	24.00	23.14	30.402	7.654	2.768	1.358

Slope (m): 2.05577
Intercept (b): -0.02807
Correlation coefficient (r): 0.99985
Uncertainty (k=2): 0.015 m^3/min

Table 2: The results of Q actual calibration data

Plate	Flow rate m^3/min	Pressure [Pa] mmHg	Temperature [Ta] °C	Temperature [Tm] °C	Ap_meter mmHg	Ap_Orifice mmHg	Y	Standard Flow [Qs] m^3/min
1	0.703	758.131	23.02	22.49	56.556	1.738	0.825	0.653
2	1.000	758.205	23.70	22.83	63.034	3.473	1.166	0.920
3	1.121	758.284	23.64	22.69	42.633	4.642	1.348	1.062
4	1.367	758.274	23.64	22.65	31.359	5.197	1.426	1.123
5	1.409	758.325	24.00	23.14	30.402	7.654	1.732	1.357

Slope (m): 1.28763
Intercept (b): -0.01756
Correlation coefficient (r): 0.99985
Uncertainty (k=2): 0.015 m^3/min

End of Certificate of Calibration



THIS CERTIFICATE REPORT MAY NOT BE REPRODUCED EXCEPT IN FULL UNLESS PERMISSION FOR REPRODUCTION IS GRANTED IN WRITING FROM THE LABORATORY

เอกสารไม่ควบคุม

เอกสารไม่ควบคุม



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
324/4 PATTANAKARN ROAD SOI 18, SUANLIANG, SUANLUANG, BANGKOK 10250
TEL.: 0-2717-3600-24 FAX: 0-2719-9484

Certificate of Calibration

Certificate No. : 25P112
Page : 1 of 2

Equipment : U-Tube Manometer

Manufacturer : Dwyer

Model : 121-36-W/M

Serial No. : -

ID No. : UAE.EFM.181/2561

Condition As-Received: Used Item

Received Date: 10 February 2025

Calibration Date: 19 February 2025

Reference: 2502-0083/WSC

Submitted by: United Analyst and Engineering Consultant Co., Ltd.

Ambient Temperature: (23 ± 2) °C

Relative Humidity: (50 ± 15) %

Atmospheric Pressure: 1012 mbar

81 Soi Udomsuk 41, Sukhumvit Road, Bangkok,
Phrakhanong, Bangkok 10260

Procedure used: The calibration was conducted by direct comparison method against Pressure Measuring Instruments Standard according to in-house calibration procedure CP-P04, using "DKD-R 6-1; Calibration of Pressure Gauges, Edition 03/2014" as a guidelines.

Condition of this result of calibration

1. Reference standards Instruments :

Instrument	Model	Serial No.	Certificate No.	Due Date
1) Pressure Calibrator	PC10GP	1189	MP-0113-24	10 Jul 2025

2. This result of calibration was made on requested at the point specified by customer.

3. Scale and conversion factor is $1 \text{ hPa} = 4.0146293 \text{ inHg}$

4. This instrument was used clean air as pressure media.

5. This instrument was installed in vertical orientation and center of connector was used as the reference level.

6. The certificate is valid only to the item calibrated on date and place of calibration.

7. This Certification is traceable to the International System of Unit maintained at:-

-National Institute of Metrology Thailand (NIMT)

Calibrated by : Nopparat Phongam
Issue Date : 21 February 2025

Approved Signatory : Attapol P.
[] Phalnoe Pratsapaipal
[] Sura Suwannasri
[x] Attapol Panurach

เอกสารไม่ควบคุม
B 0250406



Cert.No.: 25P112
Page: 2 of 2

Result of calibration: Without adjustment

Function: Pressure Measurement

Increasing Pressure

Range: 0 inHg to 36 inHg

Scale Interval: 0.1 inHg (The Fifth Estimate)

UUC Indication			AP (inHg)	Error (inHg)
Applied Pressure (inHg)	High-port side (inHg)	Low-port side (inHg)		
0.00	0.00	0.00	0.00	0.00
2.00	1.00	-0.98	1.98	-0.02
4.00	2.00	-1.98	3.98	-0.02
6.00	3.00	-3.02	6.02	0.02
8.00	4.00	-4.02	8.02	0.02
10.00	5.00	-5.04	10.04	0.04
12.00	6.00	-6.04	12.04	0.04
14.00	7.00	-7.06	14.06	0.06
16.00	8.00	-8.06	16.06	0.06
18.00	9.00	-9.06	18.06	0.06
20.00	10.00	-10.06	20.06	0.06
22.00	11.00	-11.08	22.08	0.08
24.00	12.00	-12.08	24.08	0.08
26.00	13.00	-13.10	26.10	0.10
28.00	14.00	-14.10	28.12	0.12
30.00	15.00	-15.10	30.12	0.12
32.00	16.00	-16.10	32.12	0.12
34.00	17.00	-17.08	34.10	0.10
35.50	17.86	-17.92	35.78	0.28

The uncertainty of measurement was ± 0.11 inHg

* UUC = Unit Under Calibration

* ΔP = High-port side - Low-port side

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95 %.

-o-o-

Attapol P.

เอกสารไม่ควบคุม
a 1037945



Certificate of Calibration

Certificate No.: 24P1856
Page: 1 of 2

Equipment: Aneroid Barometer

Manufacturer: Berigo

Model: -

Serial No.: -

ID No.: UAE.EMA2.110/2555

Condition As-Received: Used Item

Received Date: 24 May 2024

Calibration Date: 04 June 2024

Reference: 2405-0919WSC

Ambient Temperature: (23 ± 2) °C

Relative Humidity: (50 ± 15) %

Atmospheric Pressure: 1000 mbar

This certificate may not be reproduced other than in full,
except with the prior written approval of the head of
Corporate Services 3: Equipment Calibration and Testing Services.

Submitted by: United Analyst and Engineering Consultant Co., Ltd.

81 Soi Udomsuk 41, Sukhumvit Road,
Bangchak, Phrakhanong, Bangkok 10260

Procedure used: The calibration was conducted by direct comparison method against Pressure Measuring Instruments
Standard according to in-house calibration procedure CP-P10, using "DKD-R 6-1 : Calibration of Pressure
Gauges, Edition 03/2014" as a guidelines.

Condition of this result of calibration

1. Reference standards instruments:

Instrument	Model	Serial No.	Certificate No.	Due Date
1) Standard Barometer	DP1142	1422505048	MP-0084-24	03 May 2025

2. This instrument was installed in vertical orientation and center of the dial was used as the reference level.

3. This result of calibration was made on requested at the point specified by customer.

4. This result of calibration instrument was in absolute pressure.

5. This instrument was used clean air as pressure media.

6. The certificate is valid only to the item calibrated on date and place of calibration.

7. This Certification is traceable to the International System of Unit maintained through:-

-National Institute of Metrology Thailand (NIMT)

Calibrated by: Suksan Khankaeu
Issue Date: 06 June 2024

Approved Signatory: *Attapol P.*
[] Phalinee Prabpaijal
[] Sura Suwanasri
[x] Attapol Panurach

เอกสารไม่ควบคุม
B 0316956



Result of calibration:- Without adjustment

Function:- Absolute Pressure Measurement

Range: 720 mmHg to 800 mmHg

Scale Interval: 1 mmHg (The Fifth Estimate)

Increasing Pressure

Applied Pressure (mmHg)	720.43	730.67	740.34	751.52	756.56	761.83	773.53	798.76
UUC* Indication (mmHg)	720.0	730.0	740.0	750.0	755.0	760.0	770.0	790.0
Error (mmHg)	-0.43	-0.67	-0.34	-1.52	-1.56	-1.83	-3.53	-8.76

Decreasing Pressure

Applied Pressure (mmHg)	798.76	773.60	761.89	756.55	751.59	740.72	730.68	720.59
UUC* Indication (mmHg)	790.0	770.0	760.0	755.0	750.0	740.0	730.0	720.0
Error (mmHg)	-8.76	-3.60	-1.89	-1.55	-1.59	-0.72	-0.68	-0.59

The uncertainty of measurement was ± 0.24 mmHg

* UUC = Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied
by a coverage factor k = 2, providing a level of confidence of approximately 95 %.

-000-

Attapol P.
เอกสารไม่ควบคุม
a 1165502



Certificate of Calibration

Certificate No.: 24H1487
Page: 1 of 2

Equipment: Digital Thermo-Hygrometer

Manufacturer: Digicon

Model: TH-02A

Serial No.: 435031148

ID No.: UAE.EFM.006/2567

Condition As-Received: New Item

Received Date: 10 July 2024

Calibration Date: 15 July 2024

Reference: 2407-0383WSC

Ambient Temperature: (25 ± 3) °C

Relative Humidity: (50 ± 20) %

This certificate may not be reproduced other than in full,
except with the prior written approval of the head of
Corporate Services 3: Equipment Calibration and Testing Services.

Submitted by: United Analyst and Engineering Consultant Co., Ltd.

81 Soi Udomsuk 41, Sukhumvit Road, Bangchak,
Phrakhanong, Bangkok 10260

Procedure used: Calibration were conducted using in-house calibration procedure CP-H03 according to comparison
with standard chilled mirror sensor for humidity measurement function and comparison with standard
temperature probe for temperature measurement function into humidity / temperature chamber.

Condition of this result of calibration

1. Reference standards instruments:

Instrument	Model	Serial No.	Certificate No.	Due Date
1) Standard Chilled Mirror Hygrometer Sensor	Dew Prime II	31863	21819	25 Sep 2024
2) Handheld Thermometer With Sensor	1523	5717096	231321	08 Nov 2024

2. The certificate is valid only to the item calibrated on date and place of calibration.

3. This Certification is traceable to the International System of Unit maintained through:-

-Thunder Scientific Corporation, NVLAB Accreditation No. Calibration 200582-0

-Technology Promotion Association (Thailand-Japan), NSC-ONS Accredited No. Calibration 0008

Calibrated by: Sursat Phansudnoi
Issue Date: 17 July 2024

Approved Signatory: *Viporn*
[] Chakrit Waewwanjua
[x] Viporn Tantiyawutti
[] Unnopphol Harachai

เอกสารไม่ควบคุม



Result of Calibration:-

Function: Humidity Measurement

Reference Temperature (°C)	Standard Humidity (%R.H.)	UUC* Reading (%R.H.)	Error (%R.H.)	Uncertainty of Measurement (±%R.H.)
25.0	40.1	39	-1.1	1.4
25.0	50.1	48	-2.1	1.6
25.0	60.0	58	-2.0	1.6
25.0	70.2	68	-2.2	1.6

Result of Calibration:-

Function: Temperature Measurement

Standard Temperature (°C)	UUC* Reading (°C)	Error (°C)	Uncertainty of Measurement (±°C)
20.014	20.3	0.286	0.42
24.984	25.2	0.216	0.42
30.050	30.1	0.050	0.42
40.027	40.0	-0.027	0.42

UUC* : Unit Under Calibration

The reported uncertainty of measurement was base on standard uncertainty multiplied
by coverage factor k = 2.00, providing confidence level approximately 95%.

-000-

เอกสารไม่ควบคุม

MULTI-POINT GAS TEST REPORT


Test Date : Sep 20, 2024

Equipment : Gas Analyzer (NO₂) Model : 42i
Manufacturer : Thermo Scientific Serial Number : CM19050148

Standard Gas Concentration			Dilutor Detail	
Sulphur Dioxide (SO ₂)	42.89	PPM	Manufacturer :	Thermo Scientific
Nitric Oxide (NO)	46.77	PPM	Model :	146i
Methane (CH ₄)	-	PPM	Serial Number :	1180540071
Carbon Monoxide (CO)	965.9			
Cylinder No. :	EB0159156			
Expiration Date :	Nov 6, 2026			

Multi-point gas test data

Reference Value (ppb)			Analyzer Display (ppb)	Difference Error	Percent Error	[% Error]
Level 1	Zero	0.0	0.0	0.00	0.00	0.00
Level 2	20.00%	100.0	100.7	0.70	0.70	0.70
Level 3	40.00%	200.0	200.6	0.60	0.30	0.30
Level 4	60.00%	300.0	300.9	0.90	0.30	0.30
Level 5	80.00%	400.0	400.0	0.00	0.00	0.00
Remark : Measuring Range			500.0 ppb	Average Difference (%)		0.26

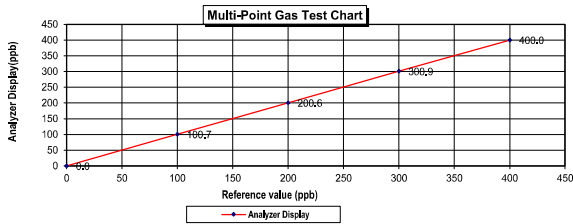

Calculate by
Sinchai C.
20 9 2567

Approve by
P. Ratanak
20 Sep 2024

MULTI-POINT GAS TEST REPORT


Test Date : Sep 17, 2024

Equipment : Gas Analyzer (NO₂) Model : 42i
Manufacturer : Thermo Scientific Serial Number : CM19050149

Standard Gas Concentration			Dilutor Detail	
Sulphur Dioxide (SO ₂)	42.89	PPM	Manufacturer :	Thermo Scientific
Nitric Oxide (NO)	46.77	PPM	Model :	146i
Methane (CH ₄)	-	PPM	Serial Number :	1180540071
Carbon Monoxide (CO)	965.9			
Cylinder No. :	EB0159156			
Expiration Date :	Nov 06, 2026			

Multi-point gas test data

Reference Value (ppb)			Analyzer Display (ppb)	Difference Error	Percent Error	[% Error]
Level 1	Zero	0.0	0.0	0.00	0.00	0.00
Level 2	20.00%	100.0	100.8	0.80	0.79	0.79
Level 3	40.00%	200.0	200.6	0.60	0.30	0.30
Level 4	60.00%	300.0	300.7	0.70	0.23	0.23
Level 5	80.00%	400.0	400.0	0.00	0.00	0.00
Remark : Measuring Range			500.0 ppb	Average Difference (%)		0.27

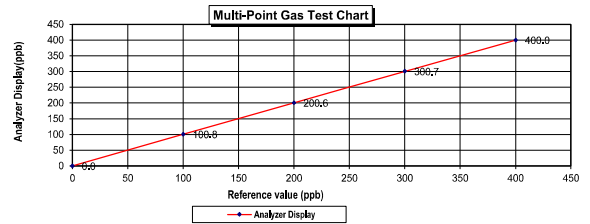

Calculate by
Sinchai C.
17 9 2567

Approve by
P. Ratanak
17 Sep 2024

MULTI-POINT GAS TEST REPORT


Test Date : Sep 26, 2024

Equipment : Gas Analyzer (NO₂) Model : 42i
Manufacturer : Thermo Scientific Serial Number : 1201778105

Standard Gas Concentration			Dilutor Detail	
Sulphur Dioxide (SO ₂)	42.89	PPM	Manufacturer :	Thermo Scientific
Nitric Oxide (NO)	46.77	PPM	Model :	146i
Methane (CH ₄)	-	PPM	Serial Number :	1180540071
Carbon Monoxide (CO)	965.9			
Cylinder No. :	EB0159156			
Expiration Date :	Nov 6, 2026			

Multi-point gas test data

Reference Value (ppb)			Analyzer Display (ppb)	Difference Error	Percent Error	[% Error]
Level 1	Zero	0.0	0.5	0.50	0.50	0.50
Level 2	20.00%	100.0	100.7	0.70	0.70	0.70
Level 3	40.00%	200.0	200.6	0.60	0.30	0.30
Level 4	60.00%	300.0	300.9	0.90	0.30	0.30
Level 5	80.00%	400.0	400.0	0.00	0.00	0.00
Remark : Measuring Range			500.0 ppb	Average Difference (%)		0.36

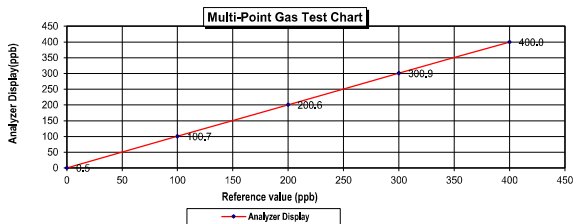

Calculate by
Sinchai C.
26 9 2567

Approve by
P. Ratanak
26 Sep 2024

MULTI-POINT GAS TEST REPORT


Test Date : Sep 20, 2024

Equipment : Gas Analyzer (NO₂) Model : 42i
Manufacturer : Thermo Scientific Serial Number : 1201778106

Standard Gas Concentration			Dilutor Detail	
Sulphur Dioxide (SO ₂)	42.89	PPM	Manufacturer :	Thermo Scientific
Nitric Oxide (NO)	46.77	PPM	Model :	146i
Methane (CH ₄)	-	PPM	Serial Number :	1180540071
Carbon Monoxide (CO)	965.9			
Cylinder No. :	EB0159156			
Expiration Date :	Nov 6, 2026			

Multi-point gas test data

Reference Value (ppb)			Analyzer Display (ppb)	Difference Error	Percent Error	[% Error]
Level 1	Zero	0.0	0.0	0.00	0.00	0.00
Level 2	20.00%	100.0	101.6	1.60	1.57	1.57
Level 3	40.00%	200.0	200.9	0.90	0.45	0.45
Level 4	60.00%	300.0	301.2	1.20	0.40	0.40
Level 5	80.00%	400.0	400.0	0.00	0.00	0.00
Remark : Measuring Range			500.0 ppb	Average Difference (%)		0.48

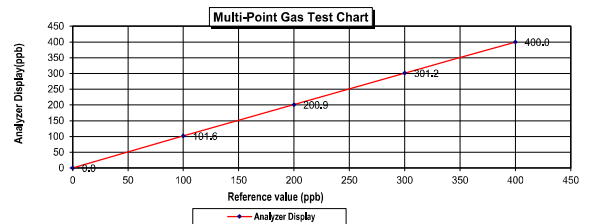

Calculate by
Sinchai C.
20 9 2567

Approve by
P. Ratanak
20 Sep 2024

CERTIFICATE OF ANALYSIS

Grade of Product: EPA PROTOCOL STANDARD

Customer: AIR LIQUIDE (THAILAND)

LTD:- E05NI91E15A0014

Part Number: E05NI91E15A0014

Cylinder Number: E05NI91E15A0014

Laboratory: 124 - Plumsteadville - PA

PGVP Number: A12023

Gas Code: CO, CO2, NO, NOX, SO2, BALN

Reference Number: 160-402772205-1

Cylinder Volume: 144.0 CF

Cylinder Pressure: 2016 PSIG

Valve Outlet: 660

Certification Date: Jul 06, 2023

Expiration Date: Jul 06, 2031

Certification performed in accordance with "EPA Traceability Protocol for Assay and Certification of Gaseous Calibration Standards" (May 2012) document EPA 800/R-12/031, using the assay procedures listed. Analytical Methodology does not require correction for analytical interference. This cylinder has a total analytical uncertainty as stated below with a confidence level of 95%. There are no significant impurities which affect the use of this calibration mixture. All concentrations are on a mole/mole basis unless otherwise noted. The results relate only to the items tested. The report shall not be reproduced except in full without approval of the laboratory. Do Not Use This Cylinder below 100 psig, i.e. 0.7 megapascals.

ANALYTICAL RESULTS

Component	Requested Concentration	Actual Concentration	Protocol Method	Total Relative Uncertainty	Assay Dates
NOX	100.0 PPM	100.4 PPM	G1	+/- 0.9% NIST Traceable	06/27/2023, 07/05/2023
NITRIC OXIDE	100.0 PPM	100.2 PPM	G1	+/- 0.9% NIST Traceable	06/27/2023, 07/05/2023
SULFUR DIOXIDE	100.0 PPM	100.0 PPM	G1	+/- 1.4% NIST Traceable	06/27/2023, 07/05/2023
CARBON MONOXIDE	200.0 PPM	199.2 PPM	G1	+/- 0.3% NIST Traceable	06/29/2023
CARBON DIOXIDE	8.000 %	7.952 %	G1	+/- 1.2% NIST Traceable	06/27/2023
NITROGEN	Balance				

CALIBRATION STANDARDS

Type	Lot ID	Cylinder No	Concentration	Uncertainty	Expiration Date
GMIS	104022308	CC754364	98.36 PPM NITRIC OXIDE/NITROGEN	+/- 0.4%	Jan 04, 2031
PRM	C2219101	APE1514048	100.19 PPM NITRIC OXIDE/NITROGEN	+/- 0.3%	Feb 28, 2025
GMIS	2023042525	CC754381	96.52 PPM NITRIC OXIDE/NITROGEN	+/- 0.4%	Apr 25, 2031
PRM	12409	D913660	15.01 PPM NITROGEN DIOXIDE/AIR	+/- 1.5%	Feb 17, 2023
GMIS	15340202002	E90130037	9.693 PPM NITROGEN DIOXIDE/NITROGEN	+/- 1.0%	Sep 29, 2025
NTRM	160102-22	KAL003620	97.69 PPM SULFUR DIOXIDE/NITROGEN	+/- 0.8%	Nov 01, 2027
CO	230601	CC745902	249.47 PPM CARBON MONOXIDE/NITROGEN	+/- 0.3%	Dec 09, 2028
NTRM	130606-02	CC411738	13.35% CARBON DIOXIDE/NITROGEN	+/- 0.6%	May 14, 2025

The SRM, NTRM, PRM, or ROD noted above is only in reference to the GMIS used in the assay and not part of the analysis.

ANALYTICAL EQUIPMENT

Instrument/Make/Model	Analytical Principle	Last Multipoint Calibration
Nicolet iS50 FTIR AUP2010245 CO2	FTIR	Jun 15, 2023
SIEMENS ULTRAMATE N1-C8-180	NDIR	Jun 14, 2023
Nicolet iS50 FTIR AUP2010245 NO	FTIR	Jun 29, 2023
Nicolet iS50 FTIR AUP2010245 NO2	FTIR	Jun 15, 2023
Nicolet iS50 FTIR AUP2010245 SO2	FTIR	Jun 08, 2023

Approved for Release

Page 1 of 1

เอกสารไม่ควบคุม

United Analyst and Engineering Consultant Co., Ltd.

3 Soi Udomsuk 41, Sukhumvit Road, Bangkok, Phrakhanong, Bangkok 10260

Tel. 0 2763 2828 Fax 0 2763 2800 www.uaeconsultant.com E-mail: uae@uaeconsultant.com

MULTI-POINT GAS TEST REPORT

Test Date : June 19, 2024


Equipment : Gas Analyzer (SO₂) Model : 43i
Manufacturer : Thermo SCIENTIFIC Serial Number : CM22387063

Standard Gas Concentration			Dilutor Detail	
Sulphur Dioxide (SO ₂)	42.89	PPM	Manufacturer :	Thermo SCIENTIFIC
Nitric Oxide (NO)	46.77	PPM	Model :	146i
Methane (CH ₄)	-	PPM	Serial Number :	1180540071
Carbon Monoxide (CO)	965.9			
Cylinder No. :	EB0159156			
Expiration Date :	Nov 06, 2026			

Multi-point gas test data

Reference Value (ppb)	Analyzer Display (ppb)	Difference Error	Percent Error	[% Error]
Level 1 Zero	0.0	0.00	0.00	0.00
Level 2 20.00%	100.0	100.8	0.80	0.79
Level 3 40.00%	200.0	200.7	0.70	0.35
Level 4 60.00%	300.0	301.1	1.10	0.37
Level 5 80.00%	400.0	400.0	0.00	0.00

Remark : Measuring Range 500.0 ppb
:Acceptable Limit $\pm 5\%$

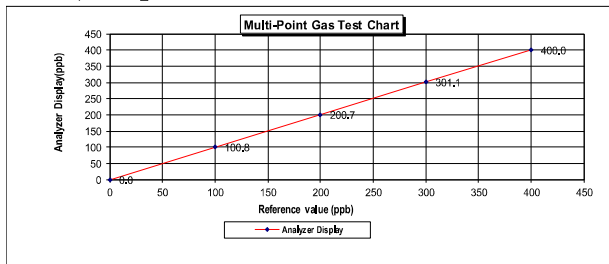

Calculate by
6/19/2024 2567

Approve by
19/June/2024

เอกสารไม่ควบคุม

United Analyst and Engineering Consultant Co., Ltd.

3 Soi Udomsuk 41, Sukhumvit Road, Bangkok, Phrakhanong, Bangkok 10260

Tel. 0 2763 2828 Fax 0 2763 2800 www.uaeconsultant.com E-mail: uae@uaeconsultant.com

MULTI-POINT GAS TEST REPORT

Test Date : Sep 6, 2024


Equipment : Gas Analyzer (SO₂) Model : 43i
Manufacturer : Thermo SCIENTIFIC Serial Number : CM22387061

Standard Gas Concentration			Dilutor Detail	
Sulphur Dioxide (SO ₂)	42.89	PPM	Manufacturer :	Thermo SCIENTIFIC
Nitric Oxide (NO)	46.77	PPM	Model :	146i
Methane (CH ₄)	-	PPM	Serial Number :	1180540071
Carbon Monoxide (CO)	965.9			
Cylinder No. :	EB0159156			
Expiration Date :	Nov 06, 2026			

Multi-point gas test data

Reference Value (ppb)	Analyzer Display (ppb)	Difference Error	Percent Error	[% Error]
Level 1 Zero	0.0	0.00	0.00	0.00
Level 2 20.00%	100.0	100.7	0.70	0.70
Level 3 40.00%	200.0	200.7	0.70	0.35
Level 4 60.00%	300.0	301.1	1.10	0.37
Level 5 80.00%	400.0	400.0	0.00	0.00

Remark : Measuring Range 500.0 ppb
:Acceptable Limit $\pm 5\%$

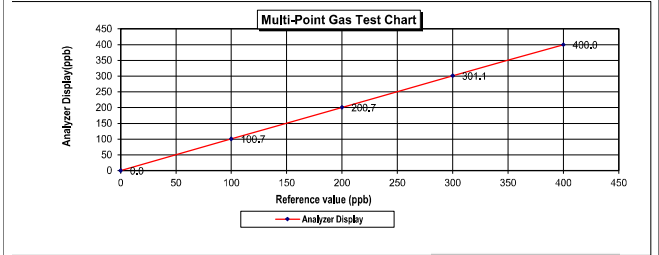

Calculate by
6/9/2024 2567

Approve by
6/Sep/2024

เอกสารไม่ควบคุม

United Analyst and Engineering Consultant Co., Ltd.

3 Soi Udomsuk 41, Sukhumvit Road, Bangkok, Phrakhanong, Bangkok 10260

Tel. 0 2763 2828 Fax 0 2763 2800 www.uaeconsultant.com E-mail: uae@uaeconsultant.com

MULTI-POINT GAS TEST REPORT

Test Date : June 19, 2024


Equipment : Gas Analyzer (SO₂) Model : 43i
Manufacturer : Thermo SCIENTIFIC Serial Number : CM22387063

Standard Gas Concentration			Dilutor Detail	
Sulphur Dioxide (SO ₂)	42.89	PPM	Manufacturer :	Thermo SCIENTIFIC
Nitric Oxide (NO)	46.77	PPM	Model :	146i
Methane (CH ₄)	-	PPM	Serial Number :	1180540071
Carbon Monoxide (CO)	965.9			
Cylinder No. :	EB0159156			
Expiration Date :	Nov 06, 2026			

Multi-point gas test data

Reference Value (ppb)	Analyzer Display (ppb)	Difference Error	Percent Error	[% Error]
Level 1 Zero	0.0	0.00	0.00	0.00
Level 2 20.00%	100.0	100.8	0.80	0.79
Level 3 40.00%	200.0	200.7	0.70	0.35
Level 4 60.00%	300.0	301.1	1.10	0.37
Level 5 80.00%	400.0	400.0	0.00	0.00

Remark : Measuring Range 500.0 ppb
:Acceptable Limit $\pm 5\%$

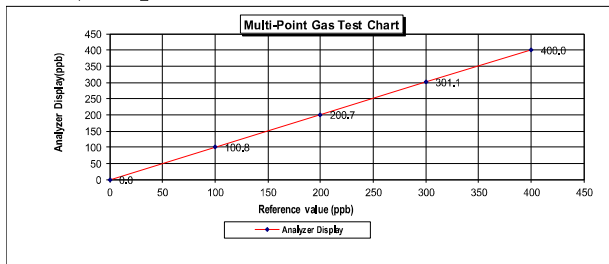

Calculate by
6/19/2024 2567

Approve by
19/June/2024

เอกสารไม่ควบคุม

United Analyst and Engineering Consultant Co., Ltd.

3 Soi Udomsuk 41, Sukhumvit Road, Bangkok, Phrakhanong, Bangkok 10260

Tel. 0 2763 2828 Fax 0 2763 2800 www.uaeconsultant.com E-mail: uae@uaeconsultant.com

MULTI-POINT GAS TEST REPORT

Test Date : Sep 4, 2024


Equipment : Gas Analyzer (SO₂) Model : 43i
Manufacturer : Thermo SCIENTIFIC Serial Number : 1201778113

Standard Gas Concentration			Dilutor Detail	
Sulphur Dioxide (SO ₂)	42.89	PPM	Manufacturer :	Thermo SCIENTIFIC
Nitric Oxide (NO)	46.77	PPM	Model :	146i
Methane (CH ₄)	-	PPM	Serial Number :	1180540071
Carbon Monoxide (CO)	965.9			
Cylinder No. :	EB0159156			
Expiration Date :	Nov 06, 2026			

Multi-point gas test data

Reference Value (ppb)	Analyzer Display (ppb)	Difference Error	Percent Error	[% Error]
Level 1 Zero	0.0	0.00	0.00	0.00
Level 2 20.00%	100.0	100.3	0.30	0.30
Level 3 40.00%	200.0	200.9	0.90	0.45
Level 4 60.00%	300.0	300.7	0.70	0.23
Level 5 80.00%	400.0	400.0	0.00	0.00

Remark : Measuring Range 500.0 ppb
:Acceptable Limit $\pm 5\%$

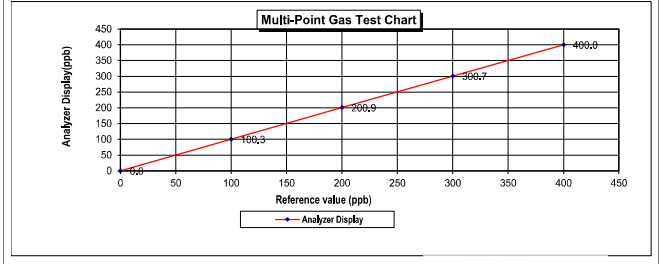

Calculate by
4/9/2024 2567

Approve by
4/Sep/2024

เอกสารไม่ควบคุม

MULTI-POINT GAS TEST REPORT


Test Date : June 19, 2024

Equipment : Gas Analyzer (SO₂) Model : 43i
Manufacturer : Thermo SCIENTIFIC Serial Number : 1201778116

Standard Gas Concentration		Dilutor Detail	
Sulphur Dioxide (SO ₂)	42.89 PPM	Manufacturer :	Thermo SCIENTIFIC
Nitric Oxide (NO)	46.77 PPM	Model :	146i
Methane (CH ₄)	- PPM	Serial Number :	1180540071
Carbon Monoxide (CO)	965.9		
Cylinder No. :	EB0159156		
Expiration Date :	Nov 06, 2025		

Multi-point gas test data

Reference Value (ppb)			Analyzer Display (ppb)	Difference Error	Percent Error	[% Error]
Level 1	Zero	0.0	0.0	0.00	0.00	0.00
Level 2	20.00%	100.0	100.5	0.50	0.50	0.50
Level 3	40.00%	200.0	201.3	1.30	0.65	0.65
Level 4	60.00%	300.0	301.7	1.70	0.56	0.56
Level 5	80.00%	400.0	400.0	0.00	0.00	0.00
Remark : Measuring Range		500.0 ppb	Average Difference (%)			0.34

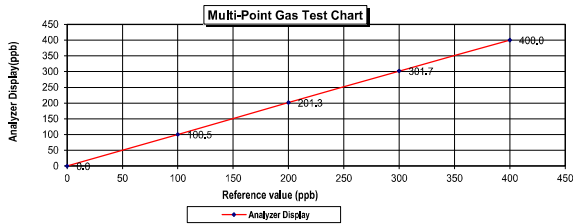

Calculate by
[Signature]
19/06/2567

Approve by
[Signature]
19/June/2024

CERTIFICATE OF ANALYSIS

Grade of Product: EPA PROTOCOL STANDARD

Customer: AIR LIQUIDE (THAILAND)
LTD :-
Part Number: E05N191E15A0014 Reference Number: 160-402772205-1
Cylinder Number: E0162121 Cylinder Volume: 144.0 CF
Laboratory: 124 - Plumsteadville - PA Cylinder Pressure: 2016 PSIG
PGVP Number: A12023 Valve Outlet: 680
Gas Code: CO,CO₂,NO,NOX,SO₂,BALN Certification Date: Jul 06, 2023

Expiration Date: Jul 06, 2031

Certification performed in accordance with EPA Traceability Protocol for Assay and Certification of Gasoline Calibration Standards (May 2012) document EPA 800/R-12/031, using the assay procedure listed. Analytical Metrology does not require correction for analytical interference. This cylinder has a total analytical uncertainty as stated below with a confidence level of 95%. There are no significant impurities which affect the use of this calibration mixture. All concentrations are on a molar basis unless otherwise noted. The results were only in the form listed. The report shall not be reproduced except in full without approval of the laboratory. Do Not Use This Cylinder below 100 psig, i.e. 0.7 megapascals.

Component	Requested Concentration	Actual Concentration	Protocol Method	Total Relative Uncertainty	Assay Dates
NOX	100.0 PPM	100.4 PPM	G1	\pm 0.9% NIST Traceable	06/27/2023, 07/06/2023
NITRIC OXIDE	100.0 PPM	100.2 PPM	G1	\pm 0.9% NIST Traceable	06/27/2023, 07/06/2023
SULFUR DIOXIDE	100.0 PPM	100.0 PPM	G1	\pm 1.4% NIST Traceable	06/27/2023, 07/06/2023
CARBON MONOXIDE	200.0 PPM	199.2 PPM	G1	\pm 0.3% NIST Traceable	06/26/2023
CARBON DIOXIDE	8.000 %	7.982 %	G1	\pm 1.2% NIST Traceable	06/27/2023
NITROGEN	Balance				

CALIBRATION STANDARDS

Type	Lot ID	Cylinder No	Concentration	Uncertainty	Expiration Date
GMIS	104202308	CC754364	98.36 PPM NITRIC OXIDE/NITROGEN	\pm 0.4%	Jan 04, 2031
PRM	C2219101	AP1514048	106.15 PPM NITRIC OXIDE/NITROGEN	\pm 0.3%	Feb 28, 2025
GMIS	2023042525	CC754381	98.52 PPM NITRIC OXIDE/NITROGEN	\pm 0.4%	Apr 25, 2031
PRM	12409	D912660	15.01 PPM NITROGEN DIOXIDE/AIR	\pm 1.5%	Feb 17, 2023
GMIS	15340020202	EB0130037	9.893 PPM NITROGEN DIOXIDE/NITROGEN	\pm 1.6%	Sep 29, 2025
NTRM	160102-22	KAL803820	97.69 PPM SULFUR DIOXIDE/NITROGEN	\pm 0.8%	Nov 01, 2027
CO	230601	CC745902	249.47 PPM CARBON MONOXIDE/NITROGEN	\pm 0.3%	Dec 09, 2028
NTRM	130805-02	CC411730	13.359 % CARBON DIOXIDE/NITROGEN	\pm 0.6%	May 14, 2025

The SRM, NTRM, PRM, or RGM noted above is only in reference to the GMS used in the assay and not part of the analysis.

ANALYTICAL EQUIPMENT

Instrument/Make/Model	Analytical Principle	Last Multi-point Calibration
Nicolet iS50 FTIR AUP2010245 CO ₂	FTIR	Jun 15, 2023
SIEMENS ULTRAMATE6E N1-C8-180	NDIR	Jun 14, 2023
Nicolet iS50 FTIR AUP2010245 NO	FTIR	Jun 29, 2023
Nicolet iS50 FTIR AUP2010245 NO ₂	FTIR	Jun 15, 2023
Nicolet iS50 FTIR AUP2010245 SO ₂	FTIR	Jun 08, 2023

[Signature]
Approved for Release

THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804, 0-2399-0469

Calibration Certificate

Issued by : Calibration & Test Section : Meteorological Instruments Bureau

Date of Issue : 3 January, 2025

Certification No. 001/25

Page : 1 of 5

Object : Wind Speed & Wind Direction Data Logger

Manufacturer : SCARLET/TECH

Type : WL-21

Mfg Code : Wireless Receiver 2111DR0072

Wind Sensor 2111DR0072

Customer : United Analyst and Engineering Consultant Co.,Ltd.

81 Soi Udomsuk 41, Sukhumvit Road,

Bangchak, Prakanong, Bangkok 10260.

Calibration Condition : Temperature 25.1 °C Barometric Pressure 1012.1 hPa

NATIONAL STANDARD WIND TUNNEL : Wind Afloat Plotting Board

: Micromanometer Theodor Friedrichs FC014 Serial No. 9310119 : HOOK GAGE NO 1425

N.I.S.T. Test Reference Number 731/241460 : Standard Velocity at 20 - 30 m/sec

: Ultrasonic Anemometer Model DA-650-3TV (sensor TR-90AH)

Serial Number 110730029 (sensor 120629586)

JAPAN QUALITY ASSURANCE ORGANIZATION : Standard Velocity at 0 - 20 m/sec

STANDARD THERMOMETER : Theodor Friedrich : Dry No.8390/94 Wet No. 8389/94

: testo, testo 545 Serial No. 02648057 : Thermoschneider No.918802

STANDARD BAROMETER : Digital Barometer Vaisala Type PTB220 No. V1220015

Digital Barometer Vaisala Type PTB220 No. V1220015

Calibrated by : *[Signature]*

Signed : *[Signature]*

(Authorised Signatory)

Mr. Watcharapol Subwat

Mr. Pisod Promsrit

for the Chief

Mechanical Engineer

Sub-Standard Instrument



THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804, 0-2399-0469

The Result of Calibration

3 January, 2025

Certification No. 001/25

Page : 2 of 5

Standard	HOOK GAGE NO. 1425			TESTED ANEMOMETER	
	Pressure	Vacuum	Velocity	Velocity	Correction
Ultrasonic Anemometer	m/sec	inches H ₂ O	inches H ₂ O	m/sec	m/sec
1.00	-	-	-	1.0	0.00
3.02	-	-	-	3.0	0.02
5.00	-	-	-	5.0	0.00
7.04	-	-	-	7.0	0.04
9.02	-	-	-	9.0	0.02
11.02	-	-	-	11.0	0.02
13.01	-	-	-	13.0	0.01
15.01	-	-	-	15.0	0.01
17.02	-	-	-	17.1	-0.08
20.02	-	-	-	20.1	-0.08

Vane Angel Bench Stand Model 18112

Young Meteorological Instruments

WIND DIRECTION	TESTED WIND DIRECTION
0	0
90	90
180	180
270	

Calibrated by : *[Signature]*

Mr. Watcharapol Subwat

Mechanical Engineer

Calibration & Test Section

Meteorological Instruments Bureau



THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804, 0-2399-0469

The Result of Calibration

Certification No. 001/25

3 January, 2025

Page : 3 of 5

Standard Barometer	Tested Barometer	Correction
Pressure	Pressure	mbar
1012.05	1012	0.05
1011.25	1011	0.25
1012.92	1013	-0.08
1010.09	1010	0.09
1008.87	1009	-0.13
1010.43	1010	0.43
1011.39	1011	0.39
1011.05	1011	0.05
1010.72	1011	-0.28
1010.30	1010	0.30
1009.81	1010	-0.19
1008.93	1009	-0.07
1009.35	1009	0.35
1009.89	1010	-0.11
1010.57	1011	-0.43
1011.41	1011	0.41
1012.31	1012	0.31
1009.75	1010	-0.25
1010.67	1011	-0.33
1011.01	1011	0.01

Average

Calibrated by :

Mr. Watcharapol Subwat
Mechanical Engineer



เอกสารไม่ควบคุม



THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804, 0-2399-0469

The Result of Calibration

Certification No. 001/25

3 January, 2025

Page : 4 of 5

Standard Barometer	Tested Barometer	Correction
Pressure	Pressure	mmHg
759.10	759	0.10
758.50	759	-0.50
769.75	760	-0.25
757.63	758	-0.37
756.71	757	-0.29
757.88	758	-0.12
758.60	759	-0.40
758.35	758	0.35
758.10	758	0.10
757.79	758	-0.21
757.42	757	0.42
756.76	757	-0.24
757.07	757	0.07
757.48	757	0.48
757.99	758	-0.01
758.62	759	-0.38
759.29	759	0.29
757.37	757	0.37
758.06	758	0.06
758.32	758	0.32

Average

Calibrated by :

Mr. Watcharapol Subwat
Mechanical Engineer



เอกสารไม่ควบคุม



THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804, 0-2399-0469

The Result of Calibration

Certification No. 001/25

3 January, 2025

Page : 5 of 5

Standard Temp. °C	Temperature Sensor Reading	
	Reading °C	Correction °C
49.5	45	0.5
30.4	30	0.4
15.6	16	-0.4

Calibrated by :

Mr. Watcharapol Subwat
Mechanical Engineer



เอกสารไม่ควบคุม



THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804, 0-2399-0469

Calibration Certificate

Issued by : Calibration & Test Section : Meteorological Instruments Bureau

Date of Issue : 3 January, 2025

Certification No. 002/25

Page : 1 of 5

Object : Wind Speed & Wind Direction Data Logger

Manufacturer : SCARLET/TECH

Type : WL-21

Mfg Code : Wireless Receiver 2205DR0113
Wind Sensor 2205DT0113

Customer : United Analyst and Engineering Consultant Co.,Ltd.
81 Soi Udomsuk 41, Sukhumvit Road,
Bangchak, Prakanong, Bangkok 10260.

Calibration Condition : Temperature 25.1 °C Barometric Pressure 1012.8 hPa

NATIONAL STANDARD WIND TUNNEL : Wind Aloft Plotting Board
: Micromanometer Theodor Friedrichs FC014 Serial No. 9310119 : HOOK GAGE NO 1425

N.I.S.T. Test Reference Number 731/241460 : Standard Velocity at 20 - 30 m/sec

: Ultrasonic Anemometer Model DA-650-3TV (sensor TR-90AH)
Serial Number 110730029 (sensor 120629586)

JAPAN QUALITY ASSURANCE ORGANIZATION : Standard Velocity at 0 - 20 m/sec

STANDARD THERMOMETER : Theodor Friedrich : Dry No.8390/94 Wet No. 8389/94

: testo, testo 645 Serial No. 02848057 : Thermoschneider No.918802

STANDARD BAROMETER : Digital Barometer Vaisala Type PTB220 No. V1220015
: Digital Barometer Vaisala Type PTB330 No. V4320001

Calibrated by :

Mr. Watcharapol Subwat
Mechanical Engineer

Signed :

Mr. Prapod Promsat

(Authorized Signatory)

For The Chief

Sub-Standard Instrument

เอกสารไม่ควบคุม



The Result of Calibration

Certification No. 002/25

Page : 3 of 5

3 January, 2025

Standard Barometer	Tested Barometer	Correction
Pressure	Pressure	mbar
1012.05	1012	0.05
1011.25	1011	0.25
1012.92	1013	-0.08
1010.09	1010	0.09
1008.87	1008	-0.13
1010.43	1010	0.43
1011.39	1011	0.39
1011.05	1011	0.05
1010.72	1011	-0.28
1010.30	1010	0.30
1009.81	1010	-0.19
1008.93	1009	-0.07
1009.35	1009	0.35
1009.89	1010	-0.11
1010.57	1011	-0.43
1011.41	1012	-0.59
1012.31	1012	0.31
1009.75	1010	-0.25
1010.67	1011	-0.33
1011.01	1011	0.01

Average

Calibrated by :

Mr. Watcharapol Subwat
Mechanical EngineerCalibration & Test Section
Meteorological Instruments Bureau

The Result of Calibration

Certification No. 002/25

Page : 2 of 5

3 January, 2025

Standard	HOOK GAGE NO. 1425			TESTED ANEMOMETER	
	Pressure	Vacuum	Velocity	Velocity	Correction
Ultrasonic Anemometer					
m/sec	inches H ₂ O	inches H ₂ O	m/sec	m/sec	m/sec
1.00	-	-	-	1.0	0.00
3.02	-	-	-	3.0	0.02
5.00	-	-	-	5.0	0.00
7.04	-	-	-	7.0	0.04
9.02	-	-	-	9.0	0.02
11.02	-	-	-	11.0	0.02
13.01	-	-	-	13.0	0.01
15.01	-	-	-	15.0	0.01
17.02	-	-	-	17.0	0.02
20.02	-	-	-	20.0	0.02

Vane Angel Bench Stand Model 18112	
Young Meteorological Instruments	
WIND DIRECTION	TESTED WIND DIRECTION
0	0
90	90
180	180
270	270

Calibrated by :
Mr. Watcharapol Subwat
Mechanical EngineerCalibration & Test Section
Meteorological Instruments Bureau

เอกสารไม่ควบคุม



The Result of Calibration

Certification No. 002/25

Page : 5 of 5

3 January, 2025

Standard	Temperature Sensor Reading	
	Reading	Correction
Temp. °C	°C	°C
45.5	45	0.5
30.4	30	0.4
15.6	15	0.6

Calibrated by :

Mr. Watcharapol Subwat
Mechanical EngineerCalibration & Test Section
Meteorological Instruments Bureau

The Result of Calibration

Certification No. 002/25

Page : 4 of 5

3 January, 2025

Standard Barometer	Tested Barometer	Correction
Pressure	Pressure	mmHg
759.10	759	0.10
758.50	759	-0.50
759.75	760	-0.25
757.63	757	0.63
756.71	757	-0.29
757.88	758	-0.12
758.60	758	0.60
758.35	758	0.35
758.10	758	0.10
757.79	758	-0.21
757.42	757	0.42
756.76	757	-0.24
757.07	757	0.07
757.48	758	-0.52
757.99	758	-0.01
758.62	759	-0.38
759.29	759	0.29
757.37	757	0.37
758.06	758	0.06
758.32	758	0.32

Average

Calibrated by :
Mr. Watcharapol Subwat
Mechanical EngineerCalibration & Test Section
Meteorological Instruments Bureau

เอกสารไม่ควบคุม

เอกสารไม่ควบคุม

MEASUREMENT RESULTS¹

The Cup anemometer, Unit Under Calibration (UUC) was exercised at 10 m/s for 5 minutes prior to calibration being performed. The standard air velocity 0.5 m/s to 5 m/s was calculated by a standard air velocity transducer which was installed 50 mm away from wind tunnel nozzle and installed 40 mm away from tip of the test section and the standard air velocity 5 m/s to 30 m/s was calculated by a pitot tube with precision differential pressure meter which was installed 50 mm away from wind tunnel nozzle and installed 40 mm away from tip of the test section. UUC was mounted on a round vertical tube of the lower plate at center of test section. The calibration was carried out under both rising and falling air velocity in the range of 1 m/s to 36 m/s at calibration interval of 1 m/s. The results of calibration and associated measurement uncertainties are reported in the table below.

V_{ref} (m/s)	Temp. wind tunnel (°C)	Temp. room (°C)	V_{UUC} (m/s)	Error (m/s)	U (k=2) (m/s)
1.093	23.98	24.05	0.9	-0.2	0.31
2.051	24.24	24.05	1.8	-0.3	0.31
3.124	24.02	24.05	2.9	-0.2	0.31
4.086	24.04	24.05	3.8	-0.3	0.31
5.09	23.68	24.05	4.9	-0.2	0.31
6.08	23.84	24.05	5.9	-0.2	0.31
6.99	23.52	24.05	6.8	-0.2	0.31
8.16	24.48	24.05	8.0	-0.2	0.31
9.12	23.50	24.05	9.1	-0.1	0.31
9.98	24.02	24.05	9.9	-0.1	0.31
11.04	23.46	24.05	11.1	0.0	0.31
12.05	23.64	24.05	12.1	0.1	0.31
13.02	23.46	24.05	13.0	-0.1	0.31
13.96	23.50	24.05	14.0	0.1	0.35
15.03	23.52	24.05	15.1	0.1	0.39
16.00	23.50	24.05	16.0	0.0	0.34

Remark:

¹ Calibration results only count for the tested circumstances and environmental conditions during which calibration took place

² Velocity of standard

³ Velocity of Unit Under Calibration

PHOTO OF CALIBRATION SET-UP



Calibration set-up of the Cup anemometer calibration in the wind tunnel of Jiranatee Associates Co., Ltd. The Cup anemometer shown may differ from the calibrated one. Remark: The proportion of the set-up is not true to scale due to imaging geometry.



MEASUREMENT ITEM
MANUFACTURER
MODEL/TYPE
SERIAL NUMBER
ID NUMBER
CONDITION AS-RECEIVED
CUSTOMER

1 Cup anemometer
1 ISI Lastem
1 Sensor: DNA202
Data logger: E-LOG
1 Sensor: BQ1705627
Data logger: 17037708
1 -
1 Used item
1 United Analyst and Engineering Consultant Co., Ltd.
81 Soi Udomsak 41, Sukhumvit Road, Bangkok,
Phraekhang, Bangkok 10260

RECEIVED DATE
MEASUREMENT DATE
ISSUE DATE

02 Aug 2024
07 Aug 2024
09 Aug 2024

ENVIRONMENTAL CONDITIONS:
Ambient condition in the laboratory are as follow:
Temperature
Relative Humidity
Atmospheric Pressure

23.0 ± 3.0 °C
55.0 ± 15.0 %RH
1010 ± 10 hPa

PLACE OF CALIBRATION

Effel-type wind tunnel of Jiranatee Associates Co., Ltd.

CALIBRATION CONDITIONS

1 Wind tunnel cross-section area¹ 900 cm²
Wind direction frontal area² 195 cm²
Diameter of mounting pipe³ - mm
Blockage ratio of test object⁴ 0.217 [-]

Preconditioning
Measurement Condition

24 hours at ambient conditions.
The average values during measurement are (23.8) °C, (41.5) %RH and (1009.0) hPa.

TABULATION OF RESULTS:
The table on next page give the measured values.

Calibrated by:
Mr. Sorawit Thachalad
Miss Jitraporn Lertsomphol

Approved signatory:
Mr. Parinya Booncharoen
Calibration Department Manager

Remark:
¹ Nipple cross-section area of the wind tunnel
² Proposed cross-section area of the tested object include mounting pipe
³ Diameter of mounting pipe
⁴ Ratio "to"

THIS CERTIFICATE OF CALIBRATION MAY NOT BE REPRODUCED EXCEPT IN FULL UNLESS PERMISSION FOR REPRODUCTION HAS BEEN OBTAINED IN WRITING FROM THE LABORATORY

เอกสารไม่ควบคุม

เอกสารไม่ควบคุม

MEASUREMENT RESULTS¹

The wind direction sensor was calibrated against standard rotary encoder by comparison method. During calibration, the measurement was carried out at 45° intervals in clockwise and counterclockwise directions after offset adjustment has been made. The flow speed of wind tunnel (usually 5 m/s) is kept constant while the sensor is rotated around its vertical axis. The results of calibration and associated measurement uncertainties are reported in the table below.

Air speed m/s	D ¹ _{max} Degree (°)	D ¹ _{min} Degree (°)	Error Degree (°)	U (k=2) Degree (°)
5.01	0.000	0	0	0.80
	45.000	46	1	0.80
	90.000	90	0	0.80
	135.000	135	0	0.80
	180.000	180	0	0.80
	225.000	225	0	0.80
	270.000	269	-1	0.80
	315.000	314	-1	0.80

Remark:

¹ Calibration results only count for the tested circumstances and environmental conditions during which calibration took place

² Direction of standard

³ Direction of Unit Under Calibration



MEASUREMENT ITEM
MANUFACTURER
MODEL/TYPE
SERIAL NUMBER
ID NUMBER
CONDITION AS-RECEIVED
CUSTOMER

1 Wind Direction Sensor
1 ISI Lastem
1 Sensor: DNA212
Data logger: E-LOG
1 Sensor: 19020250
Data logger: 17037708
1 -
1 Used item
1 United Analyst and Engineering Consultant Co., Ltd.
81 Soi Udomsak 41, Sukhumvit Road, Bangkok,
Phraekhang, Bangkok 10260

RECEIVED DATE
MEASUREMENT DATE
ISSUE DATE

02 Aug 2024
08 Aug 2024
09 Aug 2024

ENVIRONMENTAL CONDITIONS:
Ambient condition in the laboratory are as follow:
Temperature
Relative Humidity
Atmospheric Pressure

23.0 ± 3.0 °C
55.0 ± 15.0 %RH
1010 ± 10 hPa

PLACE OF CALIBRATION

Effel-type wind tunnel of Jiranatee Associates Co., Ltd.

CALIBRATION CONDITION

1 Wind tunnel cross-section area¹ 900 cm²
Wind direction frontal area² 52 cm²
Diameter of mounting pipe³ - mm
Blockage ratio of test object⁴ 0.058 [-]

Preconditioning
Measurement Condition

24 hours at ambient conditions.
The average values during measurement are (24.9) °C, (45.1) %RH and (1005.2) hPa.

TABULATION OF RESULTS:
The table on next page give the measured values.

Calibrated by:
Mr. Sorawit Thachalad
Miss Jitraporn Lertsomphol

Approved signatory:
Mr. Parinya Booncharoen
Calibration Department Manager

Remark:
¹ Nipple cross-section area of the wind tunnel
² Proposed cross-section area of the tested object include mounting pipe
³ Diameter of mounting pipe
⁴ Ratio "to"

THIS CERTIFICATE OF CALIBRATION MAY NOT BE REPRODUCED EXCEPT IN FULL UNLESS PERMISSION FOR REPRODUCTION HAS BEEN OBTAINED IN WRITING FROM THE LABORATORY

เอกสารไม่ควบคุม

เอกสารไม่ควบคุม

CERTIFICATE OF CALIBRATION

Certificate No. : CDT-180-67

Page 1 of 2 Pages

MEASUREMENT ITEM : Temperature sensor with data logger
MANUFACTURER : LSI Lastem
MODEL/TYPE : E-LDG
SERIAL NUMBER : 17037708
ID NUMBER : -
CONDITION AS-RECEIVED : New Item
CUSTOMER : United Analyst and Engineering Consultant Co., Ltd.
81 Soi Udomsuk 41, Sukhumvit Road, Bangkok,
Phrakhanong, Bangkok 10260

RECEIVED DATE : 10 Oct 2024
MEASUREMENT DATE : 21 Oct 2024
ISSUE DATE : 22 Oct 2024

ENVIRONMENTAL CONDITIONS:

Ambient condition in the laboratory are as follow:
Temperature : 23.0 ± 3.0 °C
Relative Humidity : 55.0 ± 15.0 %RH

NOTED: The certificate is valid only to the item calibrated on date and place of calibration.

TABULATION OF RESULTS:

The table on next page give the measured values.

Calibration procedure:

The temperature calibration was done by In-House calibration method as WI-CL-001 according to comparison method with standard digital temperature indicator and standard temperature probe. The temperature scale was based on ITS-90.

Traceability:

The measurement results are traceable to the International System of units (SI) through National Institute of Metrology Thailand (NIMT) Certificate number: TT-0047-24, Certificate number: ER-0101-23

Reference Used During Calibration:

1. Standard Temperature Probe
Model: STS-100 A500, Serial No.: 667682-09
2. Digital Temperature Indicator
Model: DTI-1000-A MK II, Serial No.: K71407-00593

Uncertainty of Measurement:

The reported uncertainty of measurement is based on the standard uncertainty multiplied by a coverage factor k=2, Which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty has been determined in accordance with the GUM 'Evaluation of measurement data - Guide to the expression of uncertainty in measurement'

Result of Calibration: ☐ Without Adjustment ☒ With Adjustment

Calibration Range: 20 °C to 40 °C

Function:

Table 1: This equipment was connected with temperature sensor Model: DMA672.1, S/N: 24070579.
Dimension: Diameter 14.88 mm., Length 140 mm.

Immersion Depth (mm)	Standard Reading (°C)	UUC Reading (Before) (°C)	UUC Reading (After) (°C)	Error (°C)	Uncertainty (°C)
120	20.031	18.37	19.88	-0.15	0.082
120	25.028	23.31	24.82	-0.21	0.082
120	30.016	28.20	29.72	-0.29	0.082
120	35.004	33.10	34.63	-0.37	0.082
120	39.998	38.01	39.57	-0.43	0.082

UUC*: Unit Under Calibration

End of Certificate of Calibration



Calibrated by:
☐ Mr. Sornwit Thachalad
☐ Miss Jittaporn Lertsomphol
☒ Miss Ruangrumpal Phoommit



Approved signature: Mr. Parinya Booncharoen
Calibration Department Manager

THIS CERTIFICATE MAY NOT BE REPRODUCED EXCEPT IN FULL UNLESS PERMISSION FOR REPRODUCTION HAS BEEN OBTAINED IN WRITING FROM THE LABORATORY

เอกสารไม่ควบคุม

เอกสารไม่ควบคุม

CERTIFICATE OF CALIBRATION

Certificate No. : CRT-047-67

Page 1 of 2 Pages

MEASUREMENT ITEM : Relative humidity with data logger
MANUFACTURER : LSI Lastem
MODEL/TYPE : Data Logger: E-LDG
Sensor: DMA672.1
SERIAL NUMBER : Data Logger: 17037708
Sensor: 24070579
ID NUMBER : -
CONDITION AS-RECEIVED : New Item
CUSTOMER : United Analyst and Engineering Consultant Co., Ltd.
81 Soi Udomsuk 41, Sukhumvit Road, Bangkok, Phrakhanong,
Bangkok 10260

RECEIVED DATE : 10 Oct 2024
MEASUREMENT DATE : 21 Oct 2024
ISSUE DATE : 22 Oct 2024

ENVIRONMENTAL CONDITIONS:

Ambient condition in the laboratory are as follow:
Temperature : 23.0 ± 3.0 °C
Relative Humidity : 55.0 ± 15.0 %RH

NOTED: The certificate is valid only to the item calibrated on date and place of calibration.

TABULATION OF RESULTS:

The table on next page give the measured values.

Calibration procedure:

The Relative humidity and Air Temperature calibration was done by In-House calibration method as WI-CL-001 and WI-CL-010 according to comparison method with Standard, Chilled Mirror hygrometer with Temperature sensor and standard Humidity generator chamber.

Traceability:

The measurements are traceable to the International System of units (SI) through National Institute of Metrology Thailand (NIMT) Certificate number: TH-0079-23 and Jiranatee Associates Co., Ltd. Certificate number: CDT-001-67.

Uncertainty of Measurement:

The reported uncertainty of measurement is based on the standard uncertainty multiplied by a coverage factor k=2, Which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty has been determined in accordance with the GUM 'Evaluation of measurement data - Guide to the expression of uncertainty in measurement'

Continuation of Certificate of Calibration Number: CRT-047-67

Page 2 of 2 Pages

Measurement Results:

The results of calibration and associated measurement uncertainties are reported in the table below.

Result of Calibration: ☒ Without Adjustment ☐ With Adjustment

Table 1: The results of calibration of relative humidity at 30 °C are reported in table below.

Calibration Range: 20%RH to 80%RH

Air Temperature (°C)	Standard Reading (%RH)	UUC Reading (%RH)	Error (%RH)	Uncertainty (%RH)
29.76	19.65	20.5	0.8	0.78
29.78	50.33	51.0	0.7	1.1
29.82	81.81	81.4	-0.2	2.1

UUC*: Unit Under Calibration

End of Certificate of Calibration



Calibrated by:
☐ Mr. Sornwit Thachalad
☒ Miss Jittaporn Lertsomphol
☐ Miss Ruangrumpal Phoommit



Approved signature: Mr. Parinya Booncharoen
Calibration Department Manager

THIS CERTIFICATE REPORT MAY NOT BE REPRODUCED EXCEPT IN FULL UNLESS PERMISSION FOR REPRODUCTION HAS BEEN OBTAINED IN WRITING FROM THE LABORATORY

เอกสารไม่ควบคุม

เอกสารไม่ควบคุม

CERTIFICATE OF CALIBRATION

Certificate No. : CPR-010-67

Page 1 of 2 Pages

MEASUREMENT ITEM
MANUFACTURER
MODEL/TYPE

Digital barometer
LSI Lastem
Sensor: DQA240.1
Data logger: E-LOG
Sensor: R1605260
Data logger: 17037708

SERIAL NUMBER

17037708

ID NUMBER

17037708

CONDITION AS-RECEIVED

CUSTOMER

Used item
United Analyst and Engineering Consultant Co., Ltd.
81 Soi Udomsuk 41, Sukhumvit Road, Bangkok,
Phrahanong, Bangkok 10260

RECEIVED DATE

02 Aug 2024

MEASUREMENT DATE

09 Aug 2024

ISSUE DATE

09 Aug 2024

CONDITION OF THIS RESULT OF CALIBRATION:

1. Reference Standard Instrument:

Instrument	Model	Serial No.	Certificate No.	Due Date
Absolute Pressure Transducer	CPG2500	4100126P	MP-0009-24	27 Dec 2024

2. Calibration effort for calibration sequence B

2. The UUC* was installed in vertical orientation above reference standard instrument and center of UUC* was used as the reference level.

3. Calibration conditions:

4. Condition
Pressure transmitting medium : ☒ Normal ☐ Abnormal
Air : ☐
 p_0 (20°C, 1 bar) : 1.19 kg/m³
 H_{avg} : (15±1%) %
 H_{max} : (23±3) °C
 P_{max} : (1030±10) mbar

5. The certificate is valid only to the item calibrated on date and place of calibration

Calibrated by:
☐ Mr. Sorawit Thachalad
☒ Miss Jitragorn Lertsomphol



Approved signatory:
Mr. Parinya Booncharoen
Calibration Department Manager

THIS CERTIFICATE REPORT MAY NOT BE REPRODUCED EXCEPT IN FULL UNLESS PERMISSION FOR REPRODUCTION HAS BEEN OBTAINED IN WRITING FROM THE LABORATORY

เอกสารไม่ควบคุม

CERTIFICATE OF CALIBRATION

Certificate No. : CPR-010-67

Page 2 of 2 Pages

MEASUREMENT RESULTS

☒ Without adjustment ☐ With adjustment

CALIBRATION IN THE RANGE OF : 800 mbar to 1100 mbar

The results of calibration and associated measurement uncertainties are reported in the table below.

STD (mbar)	UUC* (mbar)	Error (mbar)	Uncertainty (k=2) (mbar)
800.16	800.1	0.0	0.28
830.12	830.0	-0.1	0.28
860.13	859.9	-0.2	0.28
890.13	890.0	-0.1	0.28
920.08	920.0	0.0	0.28
950.08	949.9	-0.2	0.28
980.07	979.9	-0.2	0.28
1010.08	1010.0	-0.1	0.28
1040.07	1040.1	0.0	0.28
1070.05	1070.0	-0.1	0.28
1100.07	1100.0	-0.1	0.28

Note: UUC* Unit Under Calibration

: To convert the result in report unit to Pa should be multiply By 100

End of certificate



เอกสารไม่ควบคุม

CERTIFICATE OF CALIBRATION

Certificate No. : CPR-010-67

Page 1 of 2 Pages

MEASUREMENT ITEM
MANUFACTURER
MODEL/TYPE

Digital barometer
LSI Lastem
Sensor: DQA240.1
Data logger: E-LOG
Sensor: R1605260
Data logger: 17037708

SERIAL NUMBER

17037708

ID NUMBER

17037708

CONDITION AS-RECEIVED

CUSTOMER

Used item
United Analyst and Engineering Consultant Co., Ltd.
81 Soi Udomsuk 41, Sukhumvit Road, Bangkok,
Phrahanong, Bangkok 10260

RECEIVED DATE

02 Aug 2024

MEASUREMENT DATE

09 Aug 2024

ISSUE DATE

09 Aug 2024

CONDITION OF THIS RESULT OF CALIBRATION:

1. Reference Standard Instrument:

Instrument	Model	Serial No.	Certificate No.	Due Date
Absolute Pressure Transducer	CPG2500	4100126P	MP-0009-24	27 Dec 2024

2. Calibration effort for calibration sequence B

2. The UUC* was installed in vertical orientation above reference standard instrument and center of UUC* was used as the reference level.

3. Calibration conditions:

4. Condition
Pressure transmitting medium : ☒ Normal ☐ Abnormal
Air : ☐
 p_0 (20°C, 1 bar) : 1.19 kg/m³
 H_{avg} : (15±1%) %
 H_{max} : (23±3) °C
 P_{max} : (1030±10) mbar

5. The certificate is valid only to the item calibrated on date and place of calibration

Calibrated by:
☐ Mr. Sorawit Thachalad
☒ Miss Jitragorn Lertsomphol



Approved signatory:
Mr. Parinya Booncharoen
Calibration Department Manager

THIS CERTIFICATE REPORT MAY NOT BE REPRODUCED EXCEPT IN FULL UNLESS PERMISSION FOR REPRODUCTION HAS BEEN OBTAINED IN WRITING FROM THE LABORATORY

เอกสารไม่ควบคุม

CERTIFICATE OF CALIBRATION

Certificate No. : CPR-010-67

Page 2 of 2 Pages

MEASUREMENT RESULTS

☒ Without adjustment ☐ With adjustment

CALIBRATION IN THE RANGE OF : 600 mmHg to 825 mmHg

The results of calibration and associated measurement uncertainties are reported in the table below.

STD (mmHg)	UUC* (mmHg)	Error (mmHg)	Uncertainty (k=2) (mmHg)
600.18	600.1	0.0	0.21
622.65	622.5	-0.1	0.21
645.16	645.0	-0.2	0.21
667.66	667.6	-0.1	0.21
690.13	690.1	0.0	0.21
712.63	712.5	-0.1	0.21
735.13	735.0	-0.1	0.21
757.63	757.6	0.0	0.21
780.13	780.1	0.0	0.21
802.62	802.5	-0.1	0.21
825.14	825.1	-0.1	0.21

Note: UUC* Unit Under Calibration

: To convert the result in report unit to Pa should be multiply By 133.32

End of certificate



เอกสารไม่ควบคุม

CALIBRATION REPORT

Calibration Number : RQ-01082024
Page 1 of 2 Pages

Measurement Item : Rain gauge with data logger

Manufacturer : Data logger: LSI Lastem
Rain gauge: LSI Lastem

Model/Type : Data logger: E-LOG
Rain gauge: DGA230.1#C

Serial Number : Data logger: 17037706
Rain gauge: RQ1705209

ID NO : -

Customer : United Analyst and Engineering Consultant Co., Ltd.
81 Soi Udomsuk 41, Sukhumvit Road, Bangkok, Phraekhong, Bangkok 10260

Environmental Conditions

The measurement was carried out in an ambient temperature of (25±3)°C, and relative humidity of (50±15)%.

Measurement Method

The Rain gauge, Unit Under Calibration (UUC) was calibrated by Precision reference bottle with flow adjuster at low rate 0.6 mm per minute or 1 tipping every 20 seconds. The tipping number was determined by procedures below.

1. Obtain rain gauge inlet area

Rain gauge precise diameter in cm = Diameter/2 = R (radius)
Rain gauge area = $R^2 \times 3.14$ (UUC diameter = 20.3 cm, UUC radius = 10.15 cm)
Rain gauge area = 323.6 cm²

2. Obtain theoretical correct rain gauge answer (number of tipping) using 323.6 cm² inlet area and 0.5 L of rain.

a) 10,000 cm² / 323.6 cm² inlet area = 30.90 (rain gauge area = 1/30.90 of square meter)
b) 30.90 * 0.5 L volume = 15.45 mm (mm of rain over 1 m² surface) 500 ml of rain volume on the rain gauge area = 1545 mm of rain.
c) Number of tipping = 1545 / 0.2 mm = 77 tipping.

Note: Rain gauge is fully cleaned and leveling prior the calibration performed.

Measurement Date : Aug 08, 2023
Issued Date : Aug 09, 2023

Calibrated by:
☐ Mr. Sorawit Thachalad
☒ Miss Jitraporn Lertsomphol



Approved Signatory:

Mr. Panyia Booncharoen
Calibration Department Manager

THIS CALIBRATION REPORT MAY NOT BE REPRODUCED EXCEPT IN FULL UNLESS PERMISSION HAS BEEN OBTAINED IN WRITING FROM THE LABORATORY.

เอกสารไม่ควบคุม

เอกสารไม่ควบคุม

Jiranatee Associates Co., Ltd.
63/14-15, 67/35-36
Petchkasem 7/71, Rd. Wathapra, Bangkokkai,
Bangkok 10600 (Thailand)
Tel: +66(0)286812
Mobile: +66(0)286813
E-mail: jnac-calibration@jiranatee.com
Web site: www.jiranatee.com

Accredited calibration laboratory:
ISO/IEC 17025:2017
NSC-TIS-715 17025
CALIBRATION 0367

Air speed measurement laboratory
Calibration services department.



Certificate Number

CWS-028-67

CERTIFICATE OF CALIBRATION

Page 1 of 2 Pages

MEASUREMENT ITEM

: Cup anemometer

MANUFACTURER

: LSI Lastem

MODEL/TYPE

: Sensor: DINA202

SERIAL NUMBER

: Data logger: E-LOG

ID NUMBER

: Sensor: RQ1705209

CONDITION AS-RECEIVED

: Data logger: 17037713

CUSTOMER

: -
Used item
United Analyst and Engineering Consultant Co., Ltd.
81 Soi Udomsuk 41, Sukhumvit Road, Bangkok,
Phraekhong, Bangkok 10260

RECEIVED DATE

: 02 Aug 2024

MEASUREMENT DATE

: 07 Aug 2024

ISSUE DATE

: 09 Aug 2024

ENVIRONMENTAL CONDITIONS:

Ambient condition in the laboratory are as follow:

Temperature : 23.0 ± 3.0 °C
Relative Humidity : 55.0 ± 15.0 %RH
Atmospheric Pressure : 1030 ± 10 hPa

PLACE OF CALIBRATION

: Effel-type wind tunnel of Jiranatee Associates Co., Ltd.

CALIBRATION CONDITIONS

: Wind tunnel cross-section area¹ 900 cm²
Wind direction frontal area² 195 cm²
Diameter of mounting pipe³ - mm
Blockage ratio of test object⁴ 0.217 [-]

Preconditioning

: 24 hours at ambient conditions.

Measurement Condition

: The average values during measurement are (24.5) °C, (43.0) %RH and (1005.1) hPa.

TABULATION OF RESULTS:

The table on next page give the measured values.

Calibrated by:
☒ Mr. Sorawit Thachalad
☐ Miss Jitraporn Lertsomphol



Approved signatory:

Mr. Panyia Booncharoen
Calibration Department Manager

Remarks:

¹ Available cross-section area of the wind tunnel
² Projected cross-section area of the tested object include mounting pipe
³ Diameter of mounting pipe
⁴ Ratio 1/m²

THIS CERTIFICATE OF CALIBRATION MAY NOT BE REPRODUCED EXCEPT IN FULL UNLESS PERMISSION FOR REPRODUCTION HAS BEEN OBTAINED IN WRITING FROM THE LABORATORY

เอกสารไม่ควบคุม

Continuation of Calibration of Calibration Number

Calibration Number: RQ-01082024

Page 2 of 2 Pages

Result of Calibration: ☒ Without Adjustment ☐ With Adjustment

The results of calibration are reported in table below.

Quantity of H ₂ O (ml)	Determined Tipping	Tipping count	Acceptable Tipping count
500	77	78	75 - 79
500	77	78	75 - 79
500	77	79	75 - 79
500	77	78	75 - 79
500	77	79	75 - 79

Remark: The procedure is made to verify the correct reading of the Unit under Calibration rain gauge when a precise volume of water falls into its cone. We suggest that the number of tipping should be within ±2% difference from the 77 tipping (correct range 75-79 tipping) it means that the rain gauge meets the manufacturer acceptable limit.

End of calibration report



Page 2 of 2 Pages

MEASUREMENT RESULTS¹

The Cup anemometer, Unit Under Calibration (UUC) was exercise at 10 m/s for 5 minutes prior to calibration being performed. The standard air velocity 0.5 m/s to 5 m/s was calculated by a standard air velocity transducer which was installed 50 mm away from wind tunnel nozzle and installed 40 mm away from top of the test section and the standard air velocity 5 m/s to 30 m/s was calculated by a pilot tube with precision differential pressure meter which was installed 50 mm away from wind tunnel nozzle and installed 40 mm away from top of the test section. UUC was mounted on a round vertical tube of the lower plate at center of test section. The calibration was carried out under both rising and falling air velocity in the range of 1 m/s to 16 m/s at calibration interval of 1 m/s. The results of calibration and associated measurement uncertainties are reported in the table below.

V_{ref} (m/s)	Temp. wind tunnel (°C)	Temp. room (°C)	V_{UUC} (m/s)	Error (m/s)	U (k=2) (m/s)
1.001	24.08	24.75	0.91	-0.19	0.31
2.056	25.40	24.75	1.84	-0.22	0.31
3.148	24.10	24.75	2.91	-0.23	0.31
4.060	24.10	24.75	3.76	-0.30	0.31
5.10	23.80	24.75	4.91	-0.19	0.31
6.05	25.50	24.75	5.92	-0.13	0.31
6.99	23.90	24.75	6.83	-0.16	0.31
8.11	25.08	24.75	7.99	-0.12	0.31
9.12	24.10	24.75	9.06	-0.06	0.31
9.96	24.70	24.75	9.90	-0.06	0.31
11.05	24.20	24.75	11.05	0.00	0.31
12.01	24.52	24.75	11.97	-0.04	0.35
13.03	24.30	24.75	12.96	-0.07	0.31
13.99	24.44	24.75	13.96	-0.03	0.36
15.00	24.30	24.75	14.96	-0.04	0.37
16.01	24.30	24.75	16.02	0.01	0.34


Remark:

¹ Calibration results only count for the tested circumstances and environmental conditions during which calibration took place

² Velocity of standard

³ Velocity of Unit Under Calibration

PHOTO OF CALIBRATION SET-UP



Calibration set-up of the Cup anemometer calibration in the wind tunnel of Jiranatee Associates Co., Ltd. The Cup anemometer shown may differ from the calibrated one. Remark: The proportion of the set-up is not true to scale due to imaging geometry.



End of Certificate of Calibration

เอกสารไม่ควบคุม

MEASUREMENT RESULTS¹

The wind direction sensor was calibrated against standard rotary encoder by comparison method. During calibration, the measurement was carried out at 45° intervals in clockwise and counter-clockwise directions after offset adjustment has been made. The flow speed of wind tunnel (usually 5 m/s) is kept constant while the sensor is rotated around its vertical axis. The results of calibration and associated measurement uncertainties are reported in the table below.

Air speed	D _{meas}	D _{ref}	Error	U (k=2)
m/s	Degree (°)	Degree (°)	Degree (°)	Degree (°)
	0.000	0	0	0.80
	45.000	46	1	0.80
	90.000	91	1	0.80
	135.000	136	1	0.80
	180.000	181	1	0.80
	225.000	226	1	0.80
	270.000	270	0	0.80
	315.000	315	0	0.80

Remarks:

¹ Calibration results only count for the tested circumstances and environmental conditions during which calibration took place.

² Direction of standard

³ Direction of Unit Under Calibration

End of Certificate of Calibration



MEASUREMENT ITEM : Wind Direction Sensor
MANUFACTURER : LSI Lastem
MODEL/TYPE : Sensor: DWA212
Data logger: E-LOG
Sensor: 19050292
Data logger: 17037713
SERIAL NUMBER :
ID NUMBER :
CONDITION AS-RECEIVED :
CUSTOMER :
Used item
United Analyst and Engineering Consultant Co., Ltd.
81 Soi Udomsuk 41, Sukhumvit Road, Bangkok,
Phrakhanong, Bangkok 10260

RECEIVED DATE : 02 Aug 2024
MEASUREMENT DATE : 08 Aug 2024
ISSUE DATE : 09 Aug 2024

ENVIRONMENTAL CONDITIONS:

Ambient condition in the laboratory are as follow:

Temperature : 23.0 ± 3.0 °C
Relative Humidity : 55.0 ± 15.0 %RH
Atmospheric Pressure : 1010 ± 10 hPa

PLACE OF CALIBRATION : Eiffel-type wind tunnel of Jiranatee Associates Co., Ltd.

CALIBRATION CONDITION : Wind tunnel cross-section area¹ 900 mm²
Wind direction frontal area² 52 cm²
Diameter of mounting pipe³ mm
Blockage ratio of test object⁴ 0.058 [-]

Preconditioning : 24 hours at ambient conditions.

Measurement Condition : The average values during measurement are (24.3°C, (45.1) %RH and (1005.1) hPa.

TABULATION OF RESULTS:

The table on next page give the measured values.

Calibrated by:

☒ Mr. Sarawat Thachalad
☐ Miss Jitraporn Lertsomphol



Approved signatory:

Mr. Parinya Booncharoen
Calibration Department Manager

Remarks:

¹ Ridge cross section area of the wind tunnel.

² Projected cross section area of the tested object include mounting pipe

³ Diameter of mounting pipe

⁴ Ratio to 1

THIS CERTIFICATE OF CALIBRATION MAY NOT BE REPRODUCED EXCEPT IN FULL UNLESS PERMISSION FOR REPRODUCTION HAS BEEN OBTAINED IN WRITING FROM THE LABORATORY

เอกสารไม่ควบคุม

เอกสารไม่ควบคุม

CERTIFICATE OF CALIBRATION

Certificate No. : CDT-181-67

Page 1 of 2 Pages

MEASUREMENT ITEM : Temperature sensor with data logger
MANUFACTURER : LSI Lastem
MODEL/TYPE : E-LOG
SERIAL NUMBER : 17037713
ID NUMBER :
CONDITION AS-RECEIVED : New item
CUSTOMER :
United Analyst and Engineering Consultant Co., Ltd.
81 Soi Udomsuk 41, Sukhumvit Road, Bangkok,
Phrakhanong, Bangkok 10260

RECEIVED DATE : 10 Oct 2024
MEASUREMENT DATE : 21 Oct 2024
ISSUE DATE : 22 Oct 2024

ENVIRONMENTAL CONDITIONS:

Ambient condition in the laboratory are as follow:

Temperature : 23.0 ± 3.0 °C
Relative Humidity : 55.0 ± 15.0 %RH

NOTED: The certificate is valid only to the item calibrated on date and place of calibration.

TABULATION OF RESULTS:

The table on next page give the measured values.

Calibration procedure:

The temperature calibration was done by In-House calibration method (as WFCL-001) according to comparison method with standard digital temperature indicator and standard temperature probe. The temperature scale use was based on ITS-90.

Traceability:

The measurement results are traceable to the international system of units (SI) through National Institute of Metrology Thailand (NIMT). Certificate number: 77-0047-24. Certificate number: ER-0103-23

Reference Used During Calibration:

1. Standard Temperature Probe
Model: STS-100 AS00, Serial No.: 667682-09
2. Digital Temperature Indicator
Model: DTI-1000-A MK II, Serial No.: 671407-00591

Uncertainty of Measurement:

The reported uncertainty of measurement is based on the standard uncertainty multiplied by a coverage factor k=2. Which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty has been determined in accordance with the GUM Evaluation of measurement data - Guide to the expression of uncertainty in measurement¹

Result of Calibration: ☐ Without Adjustment ☒ With Adjustment

Calibration Range: 20 °C to 40 °C

Function:

Table 1: This equipment was connected with temperature sensor Model: DMA672.1, S/N: 24070483. Dimension: Diameter 14.88 mm., Length 140 mm.

Immersion Depth (mm)	Standard Reading (°C)	UUC Reading (Before) (°C)	UUC Reading (After) (°C)	Error (°C)	Uncertainty (°C)
120	20.021	18.38	20.27	0.35	0.082
120	25.028	23.23	25.20	0.18	0.082
120	30.015	28.11	30.14	0.02	0.082
120	35.004	33.00	35.08	0.07	0.082
120	39.995	37.89	39.99	0.00	0.082

UUC*: Unit Under Calibration

End of Certificate of Calibration



Calibrated by:

☐ Mr. Sarawat Thachalad
☐ Miss Jitraporn Lertsomphol
☒ Miss Ruangrumpai Phoornmit



Approved signatory:

Mr. Parinya Booncharoen
Calibration Department Manager

CERTIFICATE OF CALIBRATION

Certificate No. : CRT-048-67

Page 1 of 2 Pages

MEASUREMENT ITEM
MANUFACTURER : Relative humidity with data logger
MODEL/TYPE : LSI Lastem
Data Logger: E-LOG
Sensor: DMA672.1
Data Logger: 17027713
Sensor: 24070483

ID NUMBER
CONDITION AS-RECEIVED : New item
CUSTOMER : United Analyst and Engineering Consultant Co., Ltd.
81 Soi Udomsuk 41, Sukhumvit Road, Bangkok, Phrakhanong,
Bangkok 10260

RECEIVED DATE : 30 Oct 2024
MEASUREMENT DATE : 21 Oct 2024
ISSUE DATE : 22 Oct 2024

ENVIRONMENTAL CONDITIONS:

Ambient condition in the laboratory are as follow:
Temperature : 23.0 ± 3.0 °C
Relative Humidity : 55.0 ± 15.0 %RH

NOTED: The certificate is valid only to the item calibrated on date and place of calibration.

TABULATION OF RESULTS:

The table on next page give the measured values.

Calibration procedure:
The Relative humidity and Air Temperature calibration was done by in-house calibration method as WI-CI-002 and WI-CI-070 according to comparison method with Standard, Chilled Mirror hygrometer with Temperature sensor and standard Humidity generator chamber.

Traceability:
The measurements are traceable to the international system of units (SI) through National Institute of Metrology Thailand (NIMT) Certificate number: THA079-23 and Jiranatee Associates Co., Ltd. Certificate number: CDT-001-67.

Uncertainty of Measurement:
The reported uncertainty of measurement is based on the standard uncertainty multiplied by a coverage factor k=2, Which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty has been determined in accordance with the GUM 'Evaluation of measurement data - Guide to the expression of uncertainty in measurement'.

Calibrated by:
☐ Mr. Sorawit Thachalad
☒ Miss Jittrapan Lertsomphol
☐ Miss Ruangrumpal Phonmmit



Approved signatory:

Mr. Parinya Booncharoen
Calibration Department Manager

THIS CERTIFICATE REPORT MAY NOT BE REPRODUCED EXCEPT IN FULL UNLESS PERMISSION FOR REPRODUCTION HAS BEEN OBTAINED IN WRITING FROM THE LABORATORY

เอกสารไม่ควบคุม



Continuation of Certificate of Calibration Number: CRT-048-67

Page 2 of 2 Pages

Measurement Results:

The results of calibration and associated measurement uncertainties are reported in the table below.

Result of Calibration: ☒ Without Adjustment ☐ With Adjustment

Table 1: The results of calibration of relative humidity at 30 °C are reported in table below.
Calibration Range: 20%RH to 80%RH

Air Temperature (°C)	Standard Reading (%RH)	UUC Reading (%RH)	Error (%RH)	Uncertainty (%RH)
29.87	59.70	20.3	0.6	0.75
29.80	50.53	51.2	0.7	1.3
29.81	81.68	82.0	0.3	2.1

UUC*: Unit Under Calibration

End of Certificate of Calibration



Certificate No. : CPR-011-67

Page 1 of 2 Pages

MEASUREMENT ITEM
MANUFACTURER : Digital barometer
MODEL/TYPE : LSI Lastem
Sensor: DQA240.1
Data logger: E-LOG
Sensor: R1605257
Data logger: 17037713

ID NUMBER
CONDITION AS-RECEIVED : Used item
CUSTOMER : United Analyst and Engineering Consultant Co., Ltd.
81 Soi Udomsuk 41, Sukhumvit Road, Bangkok, Phrakhanong, Bangkok 10260

RECEIVED DATE : 02 Aug 2024
MEASUREMENT DATE : 09 Aug 2024
ISSUE DATE : 09 Aug 2024

CONDITION OF THIS RESULT OF CALIBRATION:

1. Reference Standard Instrument:

Instrument	Model	Serial No.	Certificate No.	Due Date
Absolute Pressure Transducer	CPG2500	410901268	MP-0009-24	27 Dec 2024

1. Calibration effort for calibration sequence B
2. The UUC* was installed in vertical orientation above reference standard instrument and center of UUC* was used as the reference level.

3. Calibration conditions:

4. Condition
Pressure transmitting medium : Air
p/h (20°C, 1 bar) : 1.19 kg/m³
T (25±15) °C : (23±1) °C
p_{amb} : (1010±10) mbar

5. The certificate is valid only to the item calibrated on date and place of calibration

Calibration procedure:
The Digital barometer was calibrated against Digital pressure calibrator, The WI-CI-003 was used as a calibration guideline.

Traceability:
The measurement results are traceable to the international system of units (SI) through the NIMT (National Metrology Institute of Thailand) with Certificate number: MP-0009-24

Uncertainty of Measurement:
The reported uncertainty of measurement is based on the standard uncertainty multiplied by a coverage factor k=2, Which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty has been determined in accordance with the GUM 'Evaluation of measurement data - Guide to the expression of uncertainty in measurement'.

Calibrated by:
☐ Mr. Sorawit Thachalad
☒ Miss Jittrapan Lertsomphol



Approved signatory:

Mr. Parinya Booncharoen
Calibration Department Manager

THIS CERTIFICATE REPORT MAY NOT BE REPRODUCED EXCEPT IN FULL UNLESS PERMISSION FOR REPRODUCTION HAS BEEN OBTAINED IN WRITING FROM THE LABORATORY

เอกสารไม่ควบคุม

CERTIFICATE OF CALIBRATION

Certificate No. : CPR-011-67

Page 2 of 2 Pages

MEASUREMENT RESULTS : ☒ Without adjustment ☐ With adjustment

CALIBRATION IN THE RANGE OF : 800 mbar to 1100 mbar

The results of calibration and associated measurement uncertainties are reported in the table below.

STD (mbar)	UUC* (mbar)	Error (mbar)	Uncertainty (k=2) (mbar)
800.15	800.1	-0.1	0.28
830.12	830.0	-0.1	0.28
860.13	860.0	-0.2	0.28
890.09	890.0	-0.1	0.28
920.11	920.1	0.0	0.28
950.10	949.9	-0.2	0.28
980.09	980.0	-0.1	0.28
1010.07	1010.0	-0.1	0.28
1040.07	1040.0	0.0	0.28
1070.06	1070.0	-0.1	0.28
1100.06	1099.8	-0.2	0.28

Note: UUC* Unit Under Calibration

: To convert the result in report unit to Pa should be multiply by 100

End of certificate



เอกสารไม่ควบคุม

เอกสารไม่ควบคุม

CERTIFICATE OF CALIBRATION

Certificate No. : CPR-011-67

Page 1 of 2 Pages

MEASUREMENT ITEM MANUFACTURER MODEL/TYPE

Digital barometer
LSI Lastem
Sensor: DQA240.1
Data logger: E-LOG
Sensor: R1605257
Data logger: 17037713

SERIAL NUMBER

-

ID NUMBER

-

CONDITION AS-RECEIVED

CUSTOMER

Used item
United Analyst and Engineering Consultant Co., Ltd.
81 Soi Udomsuk 41, Sukhumvit Road, Bangkok, Phrakhanong, Bangkok 10260

RECEIVED DATE

02 Aug 2024

MEASUREMENT DATE

09 Aug 2024

ISSUE DATE

09 Aug 2024

Calibration procedure:

The Digital barometer was calibrated against Digital pressure - calibrator, The W-CL-003 was used as a calibration guideline.

Traceability:

The measurement results are traceable to the international system of units (SI) through the NIMT (National Metrology Institute of Thailand) via Certificate number: MP-0009-24

Uncertainty of Measurement:

The reported uncertainty of measurement is based on the standard uncertainty multiplied by a coverage factor $k=2$, which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty has been determined in accordance with the GUM 'Evaluation of measurement data - Guide to the expression of uncertainty in measurement'

CONDITION OF THIS RESULT OF CALIBRATION:

1. Reference Standard Instrument:

Instrument	Model	Serial No.	Certificate No.	Due Date
Absolute Pressure Transducer	CPG2500	4100126P	MP-0009-24	27 Dec 2024

2. Calibration effort for calibration sequence B

The UUC* was installed in vertical orientation above reference standard instrument and center of UUC* was used as the reference level.

3. Calibration conditions:

4. Condition
- ☒ Normal ☐ Abnormal
- Pressure transmitting medium : Air
- p_h (20°C, 1 bar) : 1.19 kg/m³
- H_{avg} (20°C) % : (25±15) %
- T_{amb} : (23±1) °C
- P_{max} : (1030±10) mbar

5. The certificate is valid only to the item calibrated on date and place of calibration

Calibrated by:

- ☐ Mr. Sorawit Thachalad
☒ Miss Jitraporn Lertsomphol



Approved signatory:

Mr. Parinya Booncharoen
Calibration Department Manager

THIS CERTIFICATE REPORT MAY NOT BE REPRODUCED EXCEPT IN FULL UNLESS PERMISSION FOR REPRODUCTION HAS BEEN OBTAINED IN WRITING FROM THE LABORATORY

เอกสารไม่ควบคุม

CERTIFICATE OF CALIBRATION

Certificate No. : CPR-011-67

Page 2 of 2 Pages

MEASUREMENT RESULTS

☒ Without adjustment ☐ With adjustment

CALIBRATION IN THE RANGE OF

: 600 mmHg to 825 mmHg

The results of calibration and associated measurement uncertainties are reported in the table below.

STD (mmHg)	UUC* (mmHg)	Error (mmHg)	Uncertainty (k=2) (mmHg)
600.18	600.1	0.0	0.21
622.65	622.6	-0.1	0.21
645.16	645.0	-0.1	0.21
667.63	667.5	-0.1	0.21
690.15	690.1	0.0	0.21
712.65	712.5	-0.1	0.21
735.14	735.1	0.0	0.21
757.63	757.6	-0.1	0.21
780.13	780.1	0.0	0.21
802.62	802.6	-0.1	0.21
825.13	825.0	-0.1	0.21

Note: UUC* Unit Under Calibration

: To convert the result in report unit to Pa should be multiply by 133.32

End of certificate



เอกสารไม่ควบคุม

CALIBRATION REPORT

Calibration Number : R0-G1122024

Page 1 of 2 Pages

Measurement Item : Rain gauge with data logger

Manufacturer : Data logger: LSI Lastem
Rain gauge: LSI Lastem

Model/Type : Data logger: E-LOG
Rain gauge: DQA230.1

Serial Number : Data logger: 17037713
Rain gauge: 19050180

ID NO.

-

Customer

United Analyst and Engineering Consultant Co., Ltd.
81 Soi Udomsuk 41, Sukhumvit Road, Bangkok, Phrakhanong, Bangkok 10260

Environmental Condition:

The measurement was carried out in an ambient temperature of (25±3)°C and relative humidity of (50±15)%.

Measurement Method:

The Rain gauge, Unit Under Calibration (UUC) was calibrated by Precision reference bottle with flow adjuster at low rate 0.6 mm per minute or 1 tipping every 20 seconds. The tipping number was determined by procedures below.

1. Obtain rain gauge inlet area:

Rain gauge precise diameter in cm = Diameter/2 = R (radius)
Rain gauge area = $\pi R^2 \times 1.4$ (UUC diameter = 20.1 cm, UUC radius = 10.15 cm)
Rain gauge area = 323.6 cm²

2. Obtain theoretical correct rain gauge answer (number of tipping) using 323.6 cm² inlet area and 0.6 L of rain:

- a) 10,000 cm³ / 323.6 cm² inlet area = 30.90 (rain gauge area = 1/30.90 of square meter)
b) 30.90 * 0.5 L volume = 15.45 mm (mm of rain over 1 m² surface) 500 ml of rain volume on the rain gauge area = 15.45 mm of rain.
c) Number of tipping = 15.45 / 0.2 mm = 77 tipplings.

Note: Rain gauge is fully cleaned and leveling prior the calibration performed.

Measurement Date : Dec 12, 2024

Issued Date : Dec 13, 2024

Calibrated by:

- ☐ Mr. Sorawit Thachalad
☒ Miss Jitraporn Lertsomphol



Approved Signatory:

Mr. Parinya Booncharoen
Calibration Department Manager

THIS CALIBRATION REPORT MAY NOT BE REPRODUCED EXCEPT IN FULL UNLESS PERMISSION FOR REPRODUCTION HAS BEEN OBTAINED IN WRITING FROM THE LABORATORY

เอกสารไม่ควบคุม

Continuation of Calibration of Calibration Number

Calibration Number: R0-G1122024

Page 2 of 2 Pages

Result of Calibration: ☒ Without Adjustment ☐ With Adjustment

The results of calibration are reported in table below.

Quantity of H ₂ O (ml)	Determined Tipping	Tipping count	Acceptable Tipping count
500	77	77	75 - 79
500	77	76	75 - 79
500	77	76	75 - 79
500	77	76	75 - 79
500	77	76	75 - 79

Remark: The procedure is made to verify the correct reading of the Unit under Calibration rain gauge when a precise volume of water falls into its cone. We suggest that the number of tipping should be within ±2% different from the 77 tipping (correct range 75-79 tipping) it means that the rain gauge meets the manufacturer acceptable limit.

End of calibration report



เอกสารไม่ควบคุม

Certificate of Calibration

Customer

Name : UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.
Address : 81 Soi Udonsuk 41, Sukhumvit Road, Bangchak, Prakanong, Bangkok 10260

Certificate No : 24-ACT-087
Request No : Req-2024-1365

Unit Under Calibration Details

Measurement item : Acoustic Calibrator
Manufacturer : 01dB
Model : CAL31
Serial Number : 84065
ID : UAE.FM.167.2561

Class : 1
Range : 94 dB / 1000 Hz
Instrument Status : Used

Calibration Environment and Details

Temperature : (23 ±2 °C)
Humidity : (50 ± 20 %RH)
Barometric Pressure : (1013 ±10.0 hPa)
Received Date : 20 June 2024
Calibration Date : 25 June 2024
Location of Calibration : LAB 1 Acoustic
Calibration Procedure : In-house method CP-ACT-02 based on IEC 60942:2017 Electroacoustics - Sound calibrators

Reference Standard	Model	Serial Number	Traceable	Due Calibration
Sound Calibrator	SV 35A	58079	EEL	12 June 2025
THD Multimeter	2015	1047765	NIMT	16 January 2025

Traceability : This certificate provides traceability of measurement to recognized national standard, and to the realization of the international System of Units (SI).

Note :

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor $k=2$, providing a level of confidence approximately 95 %.

Calibrated By : 
Mr. Noppadon Luangart
Service Calibration Engineer

Approved By : 
Mr. Pachi Mathavorn
Calibration Engineer Supervisor

Issue Date : 25 June 2024

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Issuing Laboratory.
FM-T08-ACT-02 Rev.03 Issue date 5/6/24

เอกสารไม่ควบคุม

Certificate No : 24-ACT-087
Request No : Req-2024-1365

Sound pressure level		Calibration Results : Without Adjustment					
Calibration Range (dB)	Without Adjustment (dB)		Adjustment (dB)		Uncertainty (± dB)	Acceptance limit Class 1 (± dB)	Result
	Measured	Deviated value	Measured	Deviated value			
94 dB / 1000 Hz	93.78	-0.22	-	-	0.13	0.25	Pass

Frequency of Sound pressure level

Calibration Range (Hz)	Without Adjustment		Adjustment		Uncertainty (± %)	Acceptance limit Class 1 (± %)	Result
	Measured (Hz)	Deviated	Measured (Hz)	Deviated			
94 dB / 1000 Hz	1000.00	0.00	-	-	0.01	0.70	Pass

Total Harmonic Distortion plus Noise of Sound pressure level (THD+N %)

Calibration Range (Hz)	Without Adjustment	Adjustment	Uncertainty (± %)	Acceptance limit Class 1 (± %)	Result
	Measured (%)	Measured (%)			
94 dB / 1000 Hz	0.14	-	0.40	2.5	Pass

Note :

Function	Maximum-permitted Uncertainty of measurement
Sound pressure level	0.15 dB
Frequency	0.20%
Total distortion+noise	0.50%

- Acceptance limit was IEC60942:2017 Class 1
- The calibration results exclude the calibrator pressure correction
- The calibration results exclude the microphone volume correction

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Issuing Laboratory.
FM-T08-ACT-02 Rev.03 Issue date 5/6/24

เอกสารไม่ควบคุม

Certificate No : 24-ACT-087
Request No : Req-2024-1365

Decision Rule for Statements of Conformity


The standard decision rule employed for the statements of conformity to each calibration result will be applied using ILAC-G8:09/2019, Guidelines on the Reporting of Compliance with Specification as following Fig. and statements:

Pass - The measurement result plus the expanded uncertainty with a 95% coverage probability were within the limit.

Pass¹ - The measurement result was within the limit. However, a portion of the expanded uncertainty of measurement at 95% exceeds the limit.

Fail¹ - The measurement result was out of the limit. However, a portion of the expanded uncertainty of measurement at 95% is within the limit.

Fail - The measurement result plus the expanded uncertainty with a 95% coverage probability were outside the limit.

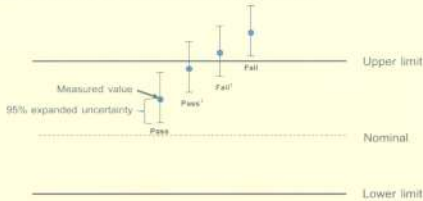

End of Calibration

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Issuing Laboratory.
FM-T08-ACT-02 Rev.03 Issue date 5/6/24

เอกสารไม่ควบคุม

Certificate of Calibration

Customer

Name : UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.
Address : 81 Soi Udonsuk 41, Sukhumvit Road, Bangchak, Prakanong, Bangkok 10260

Certificate No : 24-SLM-240
Request No : Req-2024-1459

Unit Under Calibration Details

Measurement item : Sound Level Meter
Manufacturer : Larson Davis
Model : 1xT2
Serial Number : 6005299
ID : UAE.FFM.114.2562
Resolution : 0.1 dB

Microphone Class : 2
Microphone Model : 375A04
Microphone S/N : 323471
Preamplifier Model : PRMLST2C
Preamplifier S/N : 071493
Instrument Status : Used

Calibration Environment and Details

Temperature : (23 °C ± 2 °C)
Humidity : (50 %RH ± 20 %RH)
Barometric Pressure : (1013 hPa ± 10 hPa)
Received Date : 2 July 2024
Calibrated Date : 11 July 2024
Calibration Procedure : In-house method CP-SLM-01 based on IEC 61672-1 : 2013 Electroacoustics - Sound level meters - Part 1: Periodic tests
Location of Calibration : Lab Acoustic

Reference Standard

Instrument	Brand	Model	S/N	Due calibration	Traceability
Standard Microphone	GRAS	40AN	188273	20 August 2024	GRAS
Multifrequency Calibrator	Quest	Quest-cal	EFA000234	26 July 2024	TSI
Audio Generator	Svanteck	Svsm001	131	8 October 2024	WK Electric

Note :

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor $k=2$, providing a level of confidence approximately 95 %.

Calibrated By : 
Mr. Noppadon Luangart
Service Calibration Engineer

Approved By : 
Mr. Pachi Mathavorn
Calibration Engineer Supervisor

Issue Date : 11 July 2024

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Issuing Laboratory.
FM-T08-SLM-01 Rev.04 Issue date 5/6/24

เอกสารไม่ควบคุม

Certificate No : 24-SLM-240
Request No : Req/2024-1459

1. Indication at the calibration check frequency

UUC Setting	Nominal	Before Adjust		After Adjust		UNCERTAINTY (\pm dB)	Acceptance Limit (\pm dB)	Result
FAST / A / 37-139 Calibrate Setting (dB)	Level	UUC (dB)	ERR (dB)	UUC (dB)	ERR (dB)			
1000 Hz 114 dB	113.76	115.3	1.54	113.8	+0.04	0.20	0.30	Pass

Note : Absolute sensitivity was established by the use of Sound Calibrator Brand SVANTEK, Model SV 35A, SN: 58079

2. Self-generated noise, Microphone installed

UUC Setting	Measured (dB)	UNCERTAINTY (\pm dB)
FAST / 37-139		
UUC Weighting	(dB)	(\pm dB)
A	27.1	0.10

3. Self-generated noise, Microphone replaced by the electrical input signal device

UUC Setting	Measured (dB)	UNCERTAINTY (\pm dB)
FAST / 37-139		
UUC Weighting	(dB)	(\pm dB)
A	26.6	0.10
C	26.2	0.10
Z	30.6	0.10

4. Acoustic signal test of frequency weightings (Without Windscreen)

UUC Setting	Deviation from various Frequency Weighting Response curve			UNCERTAINTY (\pm dB)	Acceptance Limit (\pm dB)	Result
	A (dB)	C (dB)	Z (dB)			
FAST / 37-139						
STD Setting	(dB)	(dB)	(dB)	(\pm dB)	(\pm dB)	
125 Hz	0.0	0.2	0.1	0.60	1.5	Pass
1000 Hz	0.0	0.0	0.0	0.60	1.0	Pass
4000 Hz	0.2	0.3	0.4	0.60	3.0	Pass
8000 Hz	-0.5	-0.4	-0.2	0.70	5.0	Pass

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the owner.
เอกสารไม่ควบคุม
FM-708-SLM-01 Rev.04 Issue date 9/6/24

Certificate No : 24-SLM-240
Request No : Req/2024-1459

5. Electrical signal test of frequency weightings, Weighting network response with relative to 1 kHz

UUC Setting	Deviation from various Frequency Weighting Response curve			UNCERTAINTY (\pm dB)	Acceptance Limit (\pm dB)	Result
FAST / 37-139	A (dB)	C (dB)	Z (dB)			
STD Setting	(dB)	(dB)	(dB)	(\pm dB)	(\pm dB)	
63 Hz	-0.2	0.0	0.0	0.20	2.0	Pass
125 Hz	-0.1	0.0	0.0		1.5	Pass
250 Hz	-0.1	0.0	0.0		1.5	Pass
500 Hz	-0.1	0.0	0.0		1.5	Pass
1000 Hz	0.0	0.0	0.0		1.0	Pass
2000 Hz	0.0	0.0	0.0		2.0	Pass
4000 Hz	0.0	-0.0	0.0		3.0	Pass
8000 Hz	0.0	0.0	0.0		5.0	Pass
16000 Hz	-0.1	-0.1	-0.1		>5, <INF	Pass

6. Frequency and time weightings at 1kHz

UUC Setting	STD	Measured		UNCERTAINTY (\pm dB)	Acceptance Limit (\pm dB)	Result
FAST / 37-139	REF	UUC (dB)	ERR (dB)			
UUC Weighting	(dB)	(dB)	(dB)	(\pm dB)	(\pm dB)	
A	114.00	114.0	0.0	0.20	0.20	Pass
C	114.00	114.0	0.0		0.20	Pass
Z	114.00	114.0	0.0		0.20	Pass

UUC Setting	STD	Measured		UNCERTAINTY (\pm dB)	Acceptance Limit (\pm dB)	Result
37-139 / A	REF	UUC (dB)	ERR (dB)			
UUC Time Response	(dB)	(dB)	(dB)	(\pm dB)	(\pm dB)	
Fast	114.00	114.0	0.0	0.20	0.10	Pass
Slow	114.00	114.0	0.0		0.10	Pass
Leq	114.00	114.0	0.0		0.10	Pass

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the owner.
เอกสารไม่ควบคุม
FM-708-SLM-01 Rev.04 Issue date 9/6/24

Certificate No : 24-SLM-240
Request No : Req/2024-1459

7. Long Term Stability

UUC Setting	Measured	UNCERTAINTY (\pm dB)	Acceptance Limit (\pm dB)	Result
FAST / A / 37-139	UUC (dB)			
STD Setting	(dB)	(\pm dB)	(\pm dB)	
Initial	114.0			
Final	114.0			
Deviated	0.0			
		0.10	0.30	Pass

8. Level linearity on the reference level range

UUC Setting	Anticipated	Deviation		UNCERTAINTY (\pm dB)	Acceptance Limit (\pm dB)	Result
FAST / A / 37-139	REF	UUC (dB)	ERR (dB)			
STD dB	(dB)	(dB)	(dB)	(\pm dB)	(\pm dB)	
139.00	139	139.0	0.0	0.30	1.1	Pass
134.00	134	134.0	0.0		1.1	Pass
129.00	129	129.0	0.0		1.1	Pass
124.00	124	124.0	0.0		1.1	Pass
119.00	119	119.0	0.0		1.1	Pass
114.00	114	114.0	0.0		1.1	Pass
109.00	109	109.0	0.0		1.1	Pass
104.00	104	104.0	0.0		1.1	Pass
99.00	99	99.0	0.0		1.1	Pass
94.00	94	94.0	0.0		1.1	Pass
89.00	89	89.0	0.0		1.1	Pass
84.00	84	84.0	0.0		1.1	Pass
79.00	79	79.0	0.0		1.1	Pass
74.00	74	74.0	0.0		1.1	Pass
69.00	69	69.0	0.0		1.1	Pass
64.00	64	64.0	0.0		1.1	Pass
59.00	59	59.0	0.0		1.1	Pass
54.00	54	54.0	0.0		1.1	Pass
49.00	49	49.0	0.0		1.1	Pass
44.00	44	44.0	0.0		1.1	Pass
39.00	39	38.2	0.2		1.1	Pass
34.00	34	34.3	0.3		1.1	Pass
29.00	29	27.4	0.4		1.1	Pass
24.00	24	24.5	0.5		1.1	Pass

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the owner.
เอกสารไม่ควบคุม
FM-708-SLM-01 Rev.04 Issue date 9/6/24

Certificate No : 24-SLM-240
Request No : Req/2024-1459

9. Level linearity including the level range control

UUC Setting	STD	Measured		UNCERTAINTY (\pm dB)	Acceptance Limit (\pm dB)	Result
FAST / A	REF	UUC (dB)	ERR (dB)			
UUC Range	(dB)	(dB)	(dB)	(\pm dB)	(\pm dB)	
37-139	41.90	42.1	0.2	0.30	1.1	Pass
	114	114.0	0.0		1.1	Pass

10. Tone burst response

UUC Setting	STD	Anticipated	Measured		UNCERTAINTY (\pm dB)	Acceptance Limit (\pm dB)	Result
A / 37-139	Toneburst	Ref	UUC (dB)	ERR (dB)			
UUC Time Response	(ms)	(dB)	(dB)	(dB)	(\pm dB)	(\pm dB)	
Fast	200	135.0	134.9	-0.1	0.20	1.0	Pass
	2	118.0	117.9	-0.1		+1.0, -2.5	Pass
	0.25	109.0	108.8	-0.2		+1.5, -5.0	Pass
Slow	200	128.6	128.5	-0.1		1.0	Pass
	2	109.0	108.9	-0.1		+1.0, -5.0	Pass
	200	129.0	129.0	0.0		1.0	Pass
SEL	2	109.0	109.1	+0.1		+1.0, -2.5	Pass
	0.25	100.0	100.0	0.0		+1.5, -5.0	Pass

11. Peak C Sound level

UUC Setting	Anticipated	Measured		UNCERTAINTY (\pm dB)	Acceptance Limit (\pm dB)	Result
FAST / C / 95-142	REF	UUC (dB)	ERR (dB)			
STD Setting	(dB)	(dB)	(dB)	(\pm dB)	(\pm dB)	
Complete cycle	137.4	136.6	-0.80	0.20	3.0	Pass
Positive half cycle	136.4	136.2	-0.20		2.0	Pass
Negative half cycle	136.4	136.2	-0.20		2.0	Pass

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the owner.
เอกสารไม่ควบคุม
FM-708-SLM-01 Rev.04 Issue date 9/6/24

Certificate No : 24-SLM-240
Request No : Req-2024-1459

12. Overload indication

UUC Setting	Measured	UNCERTAINTY	Acceptance Limit	Result
FAST / A / 37-139	UUC	(± dB)	(± dB)	
STD Setting	(dB)			
Positive one-half cycle	140.6			
Negative one-half cycle	140.7			
Deviated	-0.1	0.20	1.5	Pass

13. High Level Stability

UUC Setting	Measured	UNCERTAINTY	Acceptance Limit	Result
FAST / A / 37-139	UUC	(± dB)	(± dB)	
STD Setting	(dB)			
Initial	138.0			
Final	138.0			
Deviated	0.0	0.10	0.30	Pass

Note :

Function	Maximum-permitted Uncertainty of measurement
1. Indication at the calibration check frequency	Not applicable
2. Self-generated noise, Microphone installed	Not applicable
3. Self-generated noise, Microphone replaced by the electrical input signal device	Not applicable
4. Acoustic signal test of frequency weightings at 10 Hz to 4 kHz	0.60 dB
4. Acoustic signal test of frequency weightings at ~4 kHz to 10 kHz	0.70 dB
5. Electrical signal test of frequency weightings, Weighting network response with relative to 1 kHz	0.20 dB
6. Frequency and time weightings at 1kHz	0.20 dB
7. Long Term Stability	0.10 dB
8. Level linearity on the reference level range	0.30 dB
9. Level linearity including the level range control	0.30 dB
10. Tone burst response	0.30 dB
11. Peak C Sound level	0.35 dB
12. Overload indication	0.25 dB
13. High Level Stability	0.10 dB

Acceptance limit and Maximum-permitted Uncertainty was IEC 61672-1:2013

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of

เอกสารไม่ควบคุม
EIM-709-SLM-01 Rev.04 Issue date 3/6/24

Certificate No : 24-SLM-240
Request No : Req-2024-1459

Decision Rule for Statements of Conformity


The standard decision rule employed for the statements of conformity to each calibration result will be applied using ILAC-G8:2019: Guidelines on the Reporting of Compliance with Specification as following Fig. and statements:

Pass = The measurement result plus the expanded uncertainty with a 95% coverage probability were within the limit.

Pass¹ = The measurement result was within the limit. However, a portion of the expanded uncertainty of measurement at 95% exceeds the limit.

Fail¹ = The measurement result was out of the limit. However, a portion of the expanded uncertainty of measurement at 95% is within the limit.

Fail = The measurement result plus the expanded uncertainty with a 95% coverage probability were outside the limit.

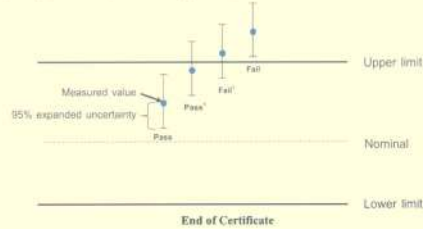

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of

เอกสารไม่ควบคุม
EIM-709-SLM-01 Rev.04 Issue date 3/6/24

Certificate of Calibration

Customer

Name : UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.
Address : 81 Soi Udomrak 41, Sukhumvit Road, Bangchak, Prakanong, Bangkok 10260

Certificate No : 24-SLM-229
Request No : Req-2024-1448

Unit Under Calibration Details

Measurement item : Microphone Class : 2
Manufacturer : Larson Davis Microphone Model : J751002
Model : LA72 Microphone S/N : 11792
Serial Number : 0005372 Pre-amplifier Model : PRMLXT2B
ID : UAE-EFM-037-2563 Pre-amplifier S/N : 056132
Resolution : 0.1 dB Instrument Status : Used

Calibration Environment and Details

Temperature : 23 °C ± 2 °C
Humidity : 50 %RH ± 20 %RH
Barometric Pressure : 1013 hPa ± 10 hPa
Received Date : 1 July 2024
Calibrated Date : 9 July 2024
Calibration Procedure : In-house method CP-SLM-01 based on IEC 61672-3 : 2013 Electroacoustics - Sound level meters - Part 3: Periodic tests
Location of Calibration : Lab Acoustic

Reference Standard

Instrument	Brand	Model	SN	Due calibration	Traceability
Standard Microphone	GRAS	40AN	188273	20 August 2024	GRAS
Multifrequency Calibrator	Quest	Quest-cal	EFA00034	26 July 2024	TSI
Audio Generator	Svantek	Svan401	131	8 October 2024	WK Electric

Note

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor k = 2, providing a level of confidence approximately 95 %.

Calibrated By : Mr. Noppalon Luangrat
Service Calibration Engineer

Approved By : Mr. Paet Mahavorn
Calibration Engineer/Supervisor
Issue Date : 9 July 2024

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of

เอกสารไม่ควบคุม
EIM-709-SLM-01 Rev.04 Issue date 3/6/24

Certificate No : 24-SLM-229
Request No : Req-2024-1448

1. Indication at the calibration check frequency

UUC Setting	Nominal	Before Adjust		After Adjust		UNCERTAINTY (± dB)	Acceptance Limit (± dB)	Result
FAST / A / 37-139	Level	UUC	ERR	UUC	ERR			
Calibrator Setting	(dB)	(dB)	(dB)	(dB)	(dB)			
1000 Hz 114 dB	113.76	114.7	0.94	113.8	-0.04	0.20	0.30	Pass

Note : Absolute sensitivity was established by the use of Sound Calibrator Brand SVANTEK, Model SV 35A, SN: 38079

2. Self-generated noise, Microphone installed

UUC Setting	Measured	UNCERTAINTY
FAST / 37-139	(dB)	(± dB)
UUC Weighting		
A	32.6	0.10

3. Self-generated noise, Microphone replaced by the electrical input signal device

UUC Setting	Measured	UNCERTAINTY
FAST / 37-139	(dB)	(± dB)
UUC Weighting		
A	31.8	0.10
C	31.7	0.10
Z	35.6	0.10

4. Acoustic signal test of frequency weightings (Without Windscreen)

UUC Setting	Deviation from various Frequency Weighting Response curve			UNCERTAINTY (± dB)	Acceptance Limit (± dB)	Result
FAST / 37-139	A	C	Z			
STD Setting	(dB)	(dB)	(dB)	(± dB)	(± dB)	
125 Hz	0.1	0.2	0.3	0.69	1.5	Pass
1000 Hz	0.0	0.0	0.0	0.69	1.0	Pass
4000 Hz	0.3	0.3	0.4	0.69	3.0	Pass
8000 Hz	0.3	0.3	0.5	0.70	5.0	Pass

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of

เอกสารไม่ควบคุม
EIM-709-SLM-01 Rev.04 Issue date 3/6/24



Certificate No : 24-SLM-229
Request No : Req-2024-1448

Page : 3/7

5. Electrical signal test of frequency weightings, Weighting network response with relative to 1 kHz

UUC Setting	Deviation from various Frequency			UNCERTAINTY	Acceptance	Result
FAST / 37-139	Weighting Response curve					
STD Setting	A (dB)	C (dB)	Z (dB)	(± dB)	Limit (± dB)	
63 Hz	-0.1	0.0	0.0	0.20	2.0	Pass
125 Hz	-0.1	0.0	0.0		1.5	Pass
250 Hz	-0.1	0.0	0.0		1.5	Pass
500 Hz	0.0	0.0	0.0		1.5	Pass
1000 Hz	0.0	0.0	0.0		1.0	Pass
2000 Hz	0.0	0.1	0.0		2.0	Pass
4000 Hz	0.0	0.0	0.0		3.0	Pass
8000 Hz	0.0	0.0	0.1		5.0	Pass
16000 Hz	0.0	0.0	0.0		+5, -INF	Pass

6. Frequency and time weightings at 1kHz

UUC Setting	STD	Measured		UNCERTAINTY (± dB)	Acceptance Limit (± dB)	Result
		UUC	ERR			
FAST / 37-139	REF					
UUC Weighting	(dB)	(dB)	(dB)			
A	114.00	114.0	0.0	0.20	0.20	Pass
C	114.00	114.0	0.0		0.20	Pass
Z	114.00	114.0	0.0		0.20	Pass

UUC Setting	STD	Measured		UNCERTAINTY (± dB)	Acceptance Limit (± dB)	Result
		UUC	ERR			
37-139 / A	REF					
UUC Time Response	(dB)	(dB)	(dB)			
Fast	114.00	114.0	0.0	0.20	0.10	Pass
Slow	114.00	114.0	0.0		0.10	Pass
Leq	114.00	114.0	0.0		0.10	Pass

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of

เอกสารไม่ควบคุม

ISO 700-01 Rev.04 Issue date 5/6/24

Certificate No : 24-SLM-229
Request No : Req-2024-1448

Page : 4/7

7. Long Term Stability

UUC Setting	Measured	UNCERTAINTY	Acceptance	Result
FAST / A / 37-139	UUC	(± dB)	Limit	
STD Setting	(dB)		(± dB)	
Initial	114.0			
Final	114.0			
Deviated	0.0	0.10	0.30	Pass

8. Level linearity on the reference level range

UUC Setting	Anticipated	Deviation		UNCERTAINTY (± dB)	Acceptance Limit (± dB)	Result
	REF	UUC	ERR			
FAST / A / 37-139	(dB)	(dB)	(dB)			
STD dB						
139.00	139	139.0	0.0	0.30	1.1	Pass
134.00	134	134.0	0.0		1.1	Pass
129.00	129	129.0	0.0		1.1	Pass
124.00	124	124.0	0.0		1.1	Pass
119.00	119	119.0	0.0		1.1	Pass
114.00	114	114.0	0.0		1.1	Pass
109.00	109	109.0	0.0		1.1	Pass
104.00	104	104.0	0.0		1.1	Pass
99.00	99	99.0	0.0		1.1	Pass
94.00	94	93.6	-0.4		1.1	Pass
89.00	89	88.6	-0.4		1.1	Pass
84.00	84	83.6	-0.4		1.1	Pass
79.00	79	78.6	-0.4		1.1	Pass
74.00	74	73.6	-0.4		1.1	Pass
69.00	69	68.6	-0.4		1.1	Pass
64.00	64	63.6	-0.4		1.1	Pass
59.00	59	58.6	-0.4		1.1	Pass
54.00	54	53.6	-0.4		1.1	Pass
49.00	49	48.7	-0.3		1.1	Pass
44.00	44	43.9	-0.1		1.1	Pass
39.00	39	39.5	0.5		1.1	Pass
34.00	34	34.9	0.9		1.1	Pass

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of

เอกสารไม่ควบคุม

ISO 700-01 Rev.04 Issue date 5/6/24



Certificate No : 24-SLM-229
Request No : Req-2024-1448

Page : 5/7

9. Level linearity including the level range control

UUC Setting	STD	Measured		UNCERTAINTY (± dB)	Acceptance Limit (± dB)	Result
		UUC	ERR			
FAST / A	REF					
UUC Range	(dB)	(dB)	(dB)			
37-139	39.10	39.6	0.5	0.20	1.1	Pass
	114	114.0	0.0		1.1	Pass

10. Tone burst response

UUC Setting	STD	Anticipated	Measured		UNCERTAINTY (± dB)	Acceptance Limit (± dB)	Result
			UUC	ERR			
A / 37-139	Toneburst	Ref	(dB)	(dB)			
UUC Time Response	(ms)						
Fast	200	135.0	135.0	0.0	0.20	1.0	Pass
	2	118.0	117.9	-0.1		+1.0, -2.5	Pass
	0.25	109.0	108.8	-0.2		+1.5, -5.0	Pass
Slow	200	128.6	128.5	-0.1		1.0	Pass
	2	109.0	108.9	-0.1		+1.0, -5.0	Pass
	200	129.0	129.0	0.0		1.0	Pass
SEL	2	109.0	109.1	+0.1		+1.0, -2.5	Pass
	0.25	100.0	100.0	0.0		+1.5, -5.0	Pass

11. Peak C Sound level

UUC Setting	Anticipated	Measured		UNCERTAINTY (± dB)	Acceptance Limit (± dB)	Result
		UUC	ERR			
FAST / C / 95-142	REF					
STD Setting	(dB)	(dB)	(dB)			
Complete cycle	137.4	136.8	-0.60	0.20	3.0	Pass
Positive half cycle	136.4	136.2	-0.20		2.0	Pass
Negative half cycle	136.4	136.2	-0.20		2.0	Pass

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of

เอกสารไม่ควบคุม

ISO 700-01 Rev.04 Issue date 5/6/24



Certificate No : 24-SLM-229
Request No : Req-2024-1448

Page : 6/7

12. Overload indication

UUC Setting	Measured	UNCERTAINTY	Acceptance	Result
FAST / A / 37-139	UUC	(± dB)	Limit	
STD Setting	(dB)		(± dB)	
Positive one-half cycle	140.7			
Negative one-half cycle	140.7			
Deviated	0.0	0.20	1.5	Pass

13. High Level Stability

UUC Setting	Measured	UNCERTAINTY	Acceptance	Result
FAST / A / 37-139	UUC	(± dB)	Limit	
STD Setting	(dB)		(± dB)	
Initial	138.0			
Final	138.0			
Deviated	0.0	0.10	0.30	Pass

Note :

Function	Maximum-permitted Uncertainty of measurement
1. Indication at the calibration check frequency	Not applicable
2. Self-generated noise, Microphone installed	Not applicable
3. Self-generated noise, Microphone replaced by the electrical input signal device	Not applicable
4. Acoustic signal test of frequency weightings at 10 Hz to 4 kHz	0.60 dB
4. Acoustic signal test of frequency weightings at >4 kHz to 10 kHz	0.70 dB
5. Electrical signal test of frequency weightings, Weighting network response with relative to 1 kHz	0.20 dB
6. Frequency and time weightings at 1kHz	0.20 dB
7. Long Term Stability	0.10 dB
8. Level linearity on the reference level range	0.30 dB
9. Level linearity including the level range control	0.30 dB
10. Tone burst response	0.30 dB
11. Peak C Sound level	0.35 dB
12. Overload indication	0.25 dB
13. High Level Stability	0.10 dB

→ Acceptance limit and Maximum-permitted Uncertainty was IEC 61872-1:2013

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of

เอกสารไม่ควบคุม


ISO 700-01 Rev.04 Issue date 5/6/24

Certificate No : 24-SLM-229
Request No : Req-2024-1448

Decision Rule for Statements of Conformity

The standard decision rule employed for the statements of conformity to each calibration result will be applied using ILAC-G8:09/2019, Guidelines on the Reporting of Compliance with Specification as following Fig. and statements

- Pass = The measurement result plus the expanded uncertainty with a 95% coverage probability were within the limit.
Fail¹ = The measurement result was within the limit. However, a portion of the expanded uncertainty of measurement at 95% exceeds the limit.
Fail² = The measurement result was out of the limit. However, a portion of the expanded uncertainty of measurement at 95% is within the limit.
Fail = The measurement result plus the expanded uncertainty with a 95% coverage probability were outside the limit.

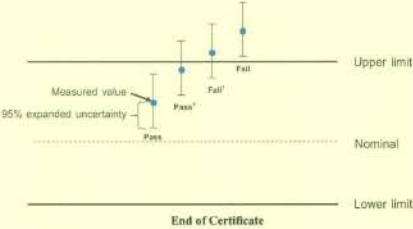

End of Certificate

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of **เอกสารไม่ควบคุม**
ISM-708-SLM-01 Rev.04 Issue date 5/6/24

Certificate of Calibration

Customer

Name : UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD. Certificate No : 24-SLM-234
Address : 81 Soi Udomsak 41, Sukhumvit Road, Bangchak, Prakanong, Bangkok Request No : Req-2024-1453
10269

Unit Under Calibration Details

Measurement item : Sound Level Meter Microphone Class : 2
Manufacturer : Larson Davis Microphone Model : 375802
Model : LX12 Microphone S/N : 011740
Serial Number : 0005286 Pre-amplifier Model : PRMLX12B
ID : UAE-FPM.102-2562 Pre-amplifier S/N : 056087
Resolution : 0.1 dB Instrument Status : Used

Calibration Environment and Details


Temperature : 23 °C ± 2 °C
Humidity : 50 %RH ± 20 %RH
Barometric Pressure : 1013 hPa ± 10 hPa
Received Date : 1 July 2024
Calibrated Date : 10 July 2024
Calibration Procedure : In-house method CP-SLM-01 based on IEC 61672-3 : 2013 Electroacoustics - Sound level meters - Part 3: Periodic tests
Location of Calibration : Lab Acoustic

Reference Standard

Instrument	Brand	Model	S/N	Due calibration	Traceability
Standard Microphone	GRAS	40AN	188273	20 August 2024	GRAS
Multifrequency Calibrator	Quest	Quest-cal	EFA000234	26 July 2024	TSI
Audio Generator	SvanteK	Svans011	131	8 October 2024	WK Electric

Note

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor k = 2, providing a level of confidence approximately 95 %.

Calibrated By : 
Mr. Noppadol Luangrat
Service Calibration Engineer

Approved By : 
Mr. Pacht Mahavorn
Calibration Engineer Supervisor
Issue Date : 10 July 2024

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of **เอกสารไม่ควบคุม**
ISM-708-SLM-01 Rev.04 Issue date 5/6/24

Certificate No : 24-SLM-234
Request No : Req-2024-1453

1. Indication at the calibration check frequency

UUC Setting	Nominal	Before Adjust		After Adjust		UNCERTAINTY (± dB)	Acceptance Limit (± dB)	Result
	Level	UUC (dB)	ERR (dB)	UUC (dB)	ERR (dB)			
FAST / A / 37-139 Calibrator Setting (dB)								
1000 Hz 114 dB	113.76	114.4	0.64	113.8	+0.04	0.20	0.30	Pass

Note : Absolute sensitivity was established by the use of Sound Calibrator Brand SVANTEK, Model SV 35A, S/N: 58079

2. Self-generated noise, Microphone installed

UUC Setting	Measured	UNCERTAINTY
FAST / 37-139		(± dB)
UUC Weighting		
A	31.3	0.10

3. Self-generated noise, Microphone replaced by the electrical input signal device

UUC Setting	Measured	UNCERTAINTY
FAST / 37-139		(± dB)
UUC Weighting		
A	31.1	0.10
C	30.6	0.10
Z	34.9	0.10

4. Acoustic signal test of frequency weightings (Without Windscreen)

UUC Setting	Deviation from various Frequency Weighting Response curve			UNCERTAINTY (± dB)	Acceptance Limit (± dB)	Result
	A	C	Z			
FAST / 37-139						
STD Setting (dB)						
125 Hz	0.0	0.1	0.1	0.60	1.5	Pass
1000 Hz	0.0	0.0	0.0	0.60	1.0	Pass
4000 Hz	1.2	1.2	1.2	0.60	3.0	Pass
8000 Hz	2.7	2.8	2.9	0.70	5.0	Pass

Certificate No : 24-SLM-234
Request No : Req-2024-1453

5. Electrical signal test of frequency weightings, Weighting network response with relative to 1 kHz

UUC Setting	Deviation from various Frequency Weighting Response curve			UNCERTAINTY (± dB)	Acceptance Limit (± dB)	Result
	A (dB)	C (dB)	Z (dB)			
FAST / 37-139						
STD Setting						
63 Hz	-0.1	0.0	0.0	0.20	2.0	Pass
125 Hz	-0.1	0.0	0.0		1.5	Pass
250 Hz	-0.1	0.0	0.0		1.5	Pass
500 Hz	0.0	0.1	0.0		1.5	Pass
1000 Hz	0.0	0.0	0.0		1.0	Pass
2000 Hz	0.0	0.1	0.0		2.0	Pass
4000 Hz	0.0	0.0	0.0		3.0	Pass
8000 Hz	0.0	0.0	0.0		5.0	Pass
16000 Hz	0.0	-0.1	-0.1		+3, -INF	Pass

6. Frequency and time weightings at 1kHz

UUC Setting	STD	Measured		UNCERTAINTY (± dB)	Acceptance Limit	Result
	REF	UUC (dB)	ERR (dB)			
FAST / 37-139						
UUC Weighting						
A	114.00	114.0	0.0	0.20	0.20	Pass
C	114.00	114.0	0.0		0.20	Pass
Z	114.00	114.0	0.0		0.20	Pass

UUC Setting	STD	Measured		UNCERTAINTY (± dB)	Acceptance Limit	Result
	REF	UUC (dB)	ERR (dB)			
37-139 / A						
UUC Time Response						
Fast	114.00	114.0	0.0	0.20	0.10	Pass
Slow	114.00	114.0	0.0		0.10	Pass
1eq	114.00	114.0	0.0		0.10	Pass

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of **เอกสารไม่ควบคุม**
ISM-708-SLM-01 Rev.04 Issue date 5/6/24

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of **เอกสารไม่ควบคุม**
ISM-708-SLM-01 Rev.04 Issue date 5/6/24

7. Long Term Stability

UUC Setting	Measured	UNCERTAINTY	Acceptance	Result
FAST / A / 37-139	UUC	(± dB)	(± dB)	
STD Setting	(dB)			
Initial	114.0			
Final	114.0			
Deviated	0.0	0.10	0.30	Pass

8. Level linearity on the reference level range

UUC Setting	Anticipated	Deviation	UNCERTAINTY	Acceptance	Result
FAST / A / 37-139	REF	UUC	ERR	Limit	
STD dB	(dB)	(dB)	(dB)	(± dB)	
136.00	139	138.0	0.0	1.1	
134.00	134	134.0	0.0	1.1	
129.00	129	129.0	0.0	1.1	Pass
124.00	124	124.0	0.0	1.1	Pass
119.00	119	119.0	0.0	1.1	Pass
114.00	114	114.0	0.0	1.1	Pass
109.00	109	109.0	0.0	1.1	Pass
104.00	104	104.0	0.0	1.1	Pass
99.00	99	99.0	0.0	1.1	Pass
94.00	94	94.0	0.0	1.1	Pass
89.00	89	89.0	0.0	1.1	Pass
84.00	84	84.0	0.0	1.1	Pass
79.00	79	79.0	0.0	1.1	Pass
74.00	74	74.0	0.0	1.1	Pass
69.00	69	69.0	0.0	1.1	Pass
64.00	64	64.0	0.0	1.1	Pass
59.00	59	59.0	0.0	1.1	Pass
54.00	54	54.0	0.0	1.1	Pass
49.00	49	48.1	0.1	1.1	Pass
44.00	44	44.2	0.2	1.1	Pass
43.00	43	43.3	0.3	1.1	Pass
42.00	42	42.3	0.3	1.1	Pass
41.00	41	41.8	0.4	1.1	Pass

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of **เอกสารไม่ควบคุม**
FSM-708-SLM-01 Rev.04 Issue date: 5/6/24

9. Level linearity including the level range control

UUC Setting	STD	Measured	UNCERTAINTY	Acceptance	Result
FAST / A	REF	UUC	ERR	Limit	
UUC Range	(dB)	(dB)	(dB)	(± dB)	
37-139	46.30	46.4	0.1	1.1	Pass
	114	114.0	0.0	1.1	Pass

10. Tone burst response

UUC Setting	STD	Anticipated	Measured	UNCERTAINTY	Acceptance	Result
A / 37-139	Toneburst	Ref	UUC	ERR	Limit	
UUC Time Response	(ms)	(dB)	(dB)	(dB)	(± dB)	
Fast	200	135.0	134.9	-0.1	1.0	Pass
	2	118.0	117.6	-0.4	+1.0, -2.5	Pass
	0.25	109.0	108.6	-0.4	+1.5, -5.0	Pass
Slow	200	128.6	128.5	-0.1	1.0	Pass
	2	109.0	108.9	-0.1	+1.0, -5.0	Pass
	200	129.0	129.0	0.0	1.0	Pass
SEL	2	109.0	109.0	0.0	+1.0, -2.5	Pass
	0.25	100.0	99.8	-0.2	+1.5, -5.0	Pass

11. Peak C Sound level

UUC Setting	Anticipated	Measured	UNCERTAINTY	Acceptance	Result
FAST / C / 95-142	REF	UUC	ERR	Limit	
STD Setting	(dB)	(dB)	(dB)	(± dB)	
Complete cycle	137.4	136.8	-0.60	2.0	Pass
Positive half cycle	136.4	136.2	-0.20	2.0	Pass
Negative half cycle	136.4	136.2	-0.20	2.0	Pass

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of **เอกสารไม่ควบคุม**
FSM-708-SLM-01 Rev.04 Issue date: 5/6/24

12. Overload indication

UUC Setting	Measured	UNCERTAINTY	Acceptance	Result
FAST / A / 37-139	UUC	(± dB)	(± dB)	
STD Setting	(dB)			
Positive one-half cycle	145.5			
Negative one-half cycle	145.4			
Deviated	0.1	0.20	1.5	Pass

13. High Level Stability

UUC Setting	Measured	UNCERTAINTY	Acceptance	Result
FAST / A / 37-139	UUC	(± dB)	(± dB)	
STD Setting	(dB)			
Initial	138.0			
Final	138.0			
Deviated	0.0	0.10	0.30	Pass

Note :

Function	Maximum-permitted Uncertainty of measurement
1. Indication at the calibration check frequency	Not applicable
2. Self-generated noise, Microphone installed	Not applicable
3. Self-generated noise, Microphone replaced by the electrical input signal device	Not applicable
4. Acoustic signal test of frequency weightings at 10 Hz to 4 kHz	0.60 dB
4. Acoustic signal test of frequency weightings at >4 kHz to 10 kHz	0.70 dB
5. Electrical signal test of frequency weightings, Weighting network response with relative to 1 kHz	0.20 dB
6. Frequency and time weightings at 1kHz	0.20 dB
7. Long Term Stability	0.10 dB
8. Level linearity on the reference level range	0.30 dB
9. Level linearity including the level range control	0.30 dB
10. Tone burst response	0.30 dB
11. Peak C Sound level	0.35 dB
12. Overload indication	0.25 dB
13. High Level Stability	0.10 dB

- Acceptance limit and Maximum-permitted Uncertainty was IEC 61672-1:2013

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of **เอกสารไม่ควบคุม**
FSM-708-SLM-01 Rev.04 Issue date: 5/6/24

Decision Rule for Statements of Conformity


The standard decision rule employed for the statements of conformity to each calibration result will be applied using ILAC-G8:09/2009, Guidelines on the Reporting of Compliance with Specification as following Fig. and statements

Pass - The measurement result plus the expanded uncertainty with a 95% coverage probability were within the limit.

Pass¹ - The measurement result was within the limit. However, a portion of the expanded uncertainty of measurement at 95% exceeds the limit.

Fail¹ - The measurement result was out of the limit. However, a portion of the expanded uncertainty of measurement at 95% is within the limit.

Fail - The measurement result plus the expanded uncertainty with a 95% coverage probability were outside the limit.

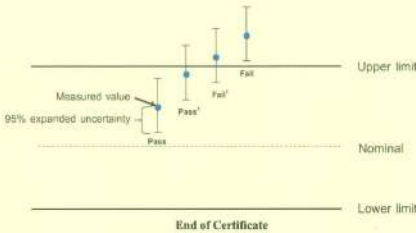

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of **เอกสารไม่ควบคุม**
FSM-708-SLM-01 Rev.04 Issue date: 5/6/24

Certificate of Calibration

Customer

Name : UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.
Address : 81 Soi Udomsak 41, Sukhumvit Road, Bangchak, Prakanong, Bangkok
10260

Certificate No : 24-SLM-238
Request No : Req-2024-1457

Unit Under Calibration Details

Measurement Item : Sound Level Meter
Manufacturer : Larson Davis
Model : LxT2
Serial Number : 0005290
ID : UAE-EM.109/2502
Resolution : 0.1 dB
Microphone Class : 2
Microphone Model : 375A04
Microphone S/N : 351837
Preamplifier Model : PRM1 sT20
Preamplifier S/N : 056077
Instrument Status : Used

Calibration Environment and Details

Temperature : 23 °C ± 2 °C
Humidity : 50 %RH ± 20 %RH
Barometric Pressure : 1013 hPa ± 10 hPa
Received Date : 2 July 2024
Calibrated Date : 11 July 2024
Calibration Procedure : In-house method CP-SLM-01 based on IEC 61672-3 : 2013 Electromagnetics - Sound level meters - Part 3: Periodic tests
Location of Calibration : Lab Acoustic


Reference Standard

Instrument	Brand	Model	SN	Due calibration	Traceability
Standard Microphone	GRAS	40AN	188273	20 August 2024	GRAS
Multifrequency Calibrator	Quest	Quest-cal	EFA000234	26 July 2024	TSI
Audio Generator	SvanteK	Svan401	131	8 October 2024	WK Electric


Note

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor $k = 2$, providing a level of confidence approximately 95%.

Calibrated By :


Mr. Noppadon Luangrit
Service Calibration Engineer

Approved By :


Mr. Pachi Mathavorn
Calibration Engineer Supervisor
Issue Date : 11 July 2024

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of

เอกสารไม่ควบคุม

FM-708-SLM-01 Rev.04 Issue date 5/8/24

Certificate No : 24-SLM-238
Request No : Req-2024-1457

1. Indication at the calibration check frequency

UUC Setting	Nominal	Before Adjust		After Adjust		UNCERTAINTY	Acceptance	Result
FAST / A / 37-139	Level	UUC	ERR	UUC	ERR	(± dB)	Limit (± dB)	
Calibrator Setting (dB)		(dB)	(dB)	(dB)	(dB)			
1000 Hz 114 dB	113.76	114.1	0.34	113.8	+0.04	0.20	0.30	Pass

Note : Absolute sensitivity was established by the use of Sound Calibrator Brand SVANTEK, Model SV 35A, SN: 58079

2. Self-generated noise, Microphone installed

UUC Setting	Measured	UNCERTAINTY
FAST / 37-139		
UUC Weighting (dB)	(dB)	(± dB)
A	25.4	0.10

3. Self-generated noise, Microphone replaced by the electrical input signal device

UUC Setting	Measured	UNCERTAINTY
FAST / 37-139		
UUC Weighting (dB)	(dB)	(± dB)
A	24.8	0.10
C	24.3	0.10
Z	28.6	0.10

4. Acoustic signal test of frequency weightings (Without Windscreen)

UUC Setting	Deviation from various Frequency Weighting Response curve			UNCERTAINTY (± dB)	Acceptance Limit (± dB)	Result
	A (dB)	C (dB)	Z (dB)			
FAST / 37-139						
STD Setting (dB)						
125 Hz	0.1	0.2	0.2	0.60	1.5	Pass
1000 Hz	0.0	0.0	0.0	0.00	1.0	Pass
4000 Hz	0.6	0.6	0.6	0.60	3.0	Pass
8000 Hz	0.8	0.8	0.9	0.70	5.0	Pass

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of

เอกสารไม่ควบคุม

FM-708-SLM-01 Rev.04 Issue date 5/8/24

Certificate No : 24-SLM-238
Request No : Req-2024-1457

5. Electrical signal test of frequency weightings, Weighting network response with relative to 1 kHz

UUC Setting	Deviation from various Frequency Weighting Response curve			UNCERTAINTY (± dB)	Acceptance Limit (± dB)	Result
	A (dB)	C (dB)	Z (dB)			
FAST / 37-139						
STD Setting (dB)						
63 Hz	-0.2	-0.1	-0.1	0.20	2.0	Pass
125 Hz	-0.1	0.0	-0.1		1.5	Pass
250 Hz	-0.1	0.0	-0.1		1.5	Pass
500 Hz	-0.1	0.0	-0.1		1.5	Pass
1000 Hz	0.0	0.0	-0.1		1.0	Pass
2000 Hz	0.0	0.0	0.0		2.0	Pass
4000 Hz	0.0	0.0	0.0		3.0	Pass
8000 Hz	-0.1	-0.1	0.0		5.0	Pass
16000 Hz	-0.1	-0.1	-0.1		+5, -INF	Pass

6. Frequency and time weightings at 1kHz

UUC Setting	STD	Measured		UNCERTAINTY (± dB)	Acceptance Limit (± dB)	Result
FAST / 37-139	REF	UUC (dB)	ERR (dB)			
UUC Weighting (dB)						
A	114.00	114.0	0.0	0.20	0.20	Pass
C	114.00	114.0	0.0		0.20	Pass
Z	114.00	114.0	0.0		0.20	Pass

UUC Setting	STD	Measured		UNCERTAINTY (± dB)	Acceptance Limit (± dB)	Result
37-139 / A	REF	UUC (dB)	ERR (dB)			
UUC Time Response (dB)						
Fast	114.00	114.0	0.0	0.20	0.10	Pass
Slow	114.00	114.0	0.0		0.10	Pass
Log	114.00	114.0	0.0		0.10	Pass

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of

เอกสารไม่ควบคุม

FM-708-SLM-01 Rev.04 Issue date 5/8/24

Certificate No : 24-SLM-238
Request No : Req-2024-1457

7. Long Term Stability

UUC Setting	Measured	UNCERTAINTY	Acceptance	Result
FAST / A / 37-139	UUC	(± dB)	Limit (± dB)	
STD Setting (dB)	(dB)			
Initial	114.0	0.10	0.30	Pass
Final	114.0			
Deviated	-0.0			

8. Level linearity on the reference level range

UUC Setting	Anticipated	Deviation		UNCERTAINTY (± dB)	Acceptance Limit (± dB)	Result
FAST / A / 37-139	REF (dB)	UUC (dB)	ERR (dB)			
STD dB						
137.00	137	137.0	0.0	0.30	1.1	Pass
134.00	134	134.0	0.0		1.1	Pass
129.00	129	129.0	0.0		1.1	Pass
124.00	124	124.0	0.0		1.1	Pass
119.00	119	119.0	0.0		1.1	Pass
114.00	114	114.0	0.0		1.1	Pass
109.00	109	109.0	0.0		1.1	Pass
104.00	104	104.0	0.0		1.1	Pass
99.00	99	99.0	0.0		1.1	Pass
94.00	94	93.9	-0.1		1.1	Pass
89.00	89	88.9	-0.1		1.1	Pass
84.00	84	83.9	-0.1		1.1	Pass
79.00	79	78.9	-0.1		1.1	Pass
74.00	74	73.9	-0.1		1.1	Pass
69.00	69	68.9	-0.1		1.1	Pass
64.00	64	63.9	-0.1		1.1	Pass
59.00	59	58.9	-0.1		1.1	Pass
54.00	54	53.9	-0.1		1.1	Pass
49.00	49	48.9	-0.1		1.1	Pass
44.00	44	44.0	0.0		1.1	Pass
39.00	39	39.3	0.3		1.1	Pass
34.00	34	34.2	0.2		1.1	Pass
29.00	29	27.2	-0.2		1.1	Pass
24.00	24	26.3	0.3		1.1	Pass
19.00	19	15.4	-0.4		1.1	Pass

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of

เอกสารไม่ควบคุม

FM-708-SLM-01 Rev.04 Issue date 5/8/24

Certificate No : 24-SLM-238
Request No : Req-2024-1457

9. Level linearity including the level range control

UUC Setting	STD	Measured		UNCERTAINTY	Acceptance Limit	Result
		UUC	ERR			
FAST / A	REF	(dB)	(dB)	(± dB)	(± dB)	
UUC Range	(dB)	(dB)	(dB)	(± dB)	(± dB)	
37-139	40.10	40.2	0.1	0.30	1.1	Pass
	114	114.0	0.0		1.1	Pass

10. Tone burst response

UUC Setting	STD	Anticipated	Measured		UNCERTAINTY	Acceptance Limit	Result
			UUC	ERR			
A / 37-139	Timeburst	Ref	(dB)	(dB)	(± dB)	(± dB)	
UUC Time Response	(ms)	(dB)	(dB)	(dB)	(± dB)	(± dB)	
Fast	200	135.0	135.0	0.0	0.20	1.0	Pass
	2	118.0	117.9	-0.1		+1.0, -2.5	Pass
	0.25	109.0	108.8	-0.4		+1.5, -5.0	Pass
Slow	200	128.6	128.5	-0.1		1.0	Pass
	2	109.0	108.9	-0.1		+1.0, -5.0	Pass
	200	129.0	129.0	0.0		1.0	Pass
SEL	2	109.0	109.0	0.0	0.20	+1.0, -2.5	Pass
	0.25	100.0	99.8	-0.2		+1.5, -5.0	Pass

11. Peak C Sound level

UUC Setting	Anticipated	Measured		UNCERTAINTY	Acceptance	Result
FAST / C / 95-142	REF	UUC	ERR		Limit	
STD Setting	(dB)	(dB)	(dB)	(± dB)	(± dB)	
Complete cycle	137.4	136.6	-0.80	0.20	3.0	Pass
Positive half cycle	136.4	136.2	-0.20		2.0	Pass
Negative half cycle	136.4	136.2	-0.20		2.0	Pass

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of

เอกสารไม่ควบคุม

FM-708-SLM-01 Rev.04 Issue date 5/6/24

Certificate No : 24-SLM-238
Request No : Req-2024-1457

12. Overload indication

UUC Setting	Measured	UNCERTAINTY	Acceptance Limit	Result
FAST / A / 37-139	UUC			
STD Setting	(dB)	(± dB)	(± dB)	
Positive one-half cycle	138.8	0.20	1.5	Pass
Negative one-half cycle	138.7			
Deviated	0.1	0.20	1.5	Pass

13. High Level Stability

UUC Setting	Measured	UNCERTAINTY	Acceptance Limit	Result
FAST / A / 37-139	UUC			
STD Setting	(dB)	(± dB)	(± dB)	
Initial	138.0	0.10	0.30	Pass
Final	138.0			
Deviated	0.0	0.10	0.30	Pass

Note :

Function	Maximum-permitted Uncertainty of measurement
1. Indication at the calibration check frequency	Not applicable
2. Self-generated noise, Microphone installed	Not applicable
3. Self-generated noise, Microphone replaced by the electrical input signal device	Not applicable
4. Acoustic signal test of frequency weightings at 10 Hz to 4 kHz	0.60 dB
4. Acoustic signal test of frequency weightings at ~4 kHz to 10 kHz	0.70 dB
5. Electrical signal test of frequency weightings, Weighting network response with relative to 1 kHz	0.20 dB
6. Frequency and time weightings at 1 kHz	0.20 dB
7. Long Term Stability	0.10 dB
8. Level linearity on the reference level range	0.30 dB
9. Level linearity including the level range control	0.30 dB
10. Tone burst response	0.30 dB
11. Peak C Sound level	0.35 dB
12. Overload indication	0.25 dB
13. High Level Stability	0.10 dB

> Acceptance limit and Maximum-permitted Uncertainty was IEC 61672-1:2013

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of

เอกสารไม่ควบคุม

FM-708-SLM-01 Rev.04 Issue date 5/6/24

Certificate No : 24-SLM-238
Request No : Req-2024-1457

Decision Rule for Statements of Conformity


The standard decision rule employed for the statements of conformity to each calibration result will be applied using ILAC-G8:08-2019: Guidelines on the Reporting of Compliance with Specification as following Fig. and statements

Pass - The measurement result plus the expanded uncertainty with a 95% coverage probability were within the limits

Pass¹ - The measurement result was within the limit. However, a portion of the expanded uncertainty of measurement at 95% exceeds the limit

Fail¹ - The measurement result was not of the limit. However, a portion of the expanded uncertainty of measurement at 95% is within the limit.

Fail - The measurement result plus the expanded uncertainty with a 95% coverage probability were outside the limit.

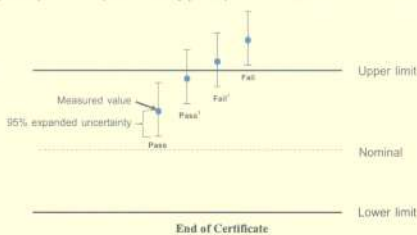

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of

เอกสารไม่ควบคุม

FM-708-SLM-01 Rev.04 Issue date 5/6/24

Certificate of Calibration

Customer

Name : UNITED ANALYST AND ENGINEERING CONSULTANT CO., LTD.
Address : 81 Soi Udomsak 41, Sukhumvit Road, Bangchak, Prakanong, Bangkok 10260

Certificate No : 24-SLM-231
Request No : Req-2024-1450

Unit Under Calibration Details

Measurement Item : Sound Level Meter
Manufacturer : Larson Davis
Model : LXT2
Serial Number : 0005293
ID : UAE-EFM1982562
Resolution : 0.1 dB
Microphone Class : 2
Microphone Model : 375B02
Microphone S/N : 11792
Preamplifier Model : PRM1.x12B
Preamplifier S/N : 056073
Instrument Status : Used

Calibration Environment and Details


Temperature : 23 °C ± 2 °C
Humidity : 50 %RH ± 20 %RH
Barometric Pressure : 1013 hPa ± 10 hPa
Received Date : 1 July 2024
Calibrated Date : 10 July 2024
Calibration Procedure : In-house method CP-SLM-01 based on IEC 61672-3: 2013 Electroacoustics – Sound level meters – Part 3: Periodic tests
Location of Calibration : Lab Acoustic

Reference Standard

Instrument	Brand	Model	SN	Due calibration	Traceability
Standard Microphone	GRAS	40AN	188273	20 August 2024	GRAS
Multi-frequency Calibrator	Quest	Quest-cal	EFA000254	26 July 2024	TSI
Audio Generator	Svante	Svan401	131	8 October 2024	WK Electric

Note

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor $k = 2$, providing a level of confidence approximately 95 %.

Calibrated By : 
Mr. Noppadon Luangrit
Service Calibration Engineer

Approved By : 
Mr. Paat Mahavorn
Calibration Engineer Supervisor
Issue Date : 10 July 2024

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of

เอกสารไม่ควบคุม

FM-708-SLM-01 Rev.04 Issue date 5/6/24

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of

เอกสารไม่ควบคุม

FM-708-SLM-01 Rev.04 Issue date 5/6/24

Certificate No : 24-SLM-231
Request No : Req-2024-1458

1. Indication at the calibration check frequency

UUC Setting	Nominal	Before Adjust		After Adjust		UNCERTAINTY (± dB)	Acceptance Limit (± dB)	Result
		UUC (dB)	ERR (dB)	UUC (dB)	ERR (dB)			
FAST / A / 37-139	Level							
Calibrator Setting (dB)		(dB)		(dB)				
1000 Hz 114 dB	113.76	114.3	0.54	113.8	+0.04	0.20	0.30	Pass

Note : Absolute sensitivity was established by the use of Sound Calibrator Brand SVANTEK, Model SV 35A, SN. 58079

2. Self-generated noise, Microphone installed

UUC Setting	Measured (dB)	UNCERTAINTY (± dB)
FAST / 37-139		
UUC Weighting		
A	29.8	0.10

3. Self-generated noise, Microphone replaced by the electrical input signal device

UUC Setting	Measured (dB)	UNCERTAINTY (± dB)
FAST / 37-139		
UUC Weighting		
A	29.4	0.10
C	28.8	0.10
Z	32.9	0.10

4. Acoustic signal test of frequency weightings (Without Windscreen)

UUC Setting	Deviation from various Frequency Weighting Response curve			UNCERTAINTY (± dB)	Acceptance Limit (± dB)	Result
	A	C	Z			
FAST / 37-139						
STD Setting (dB)	(dB)	(dB)	(dB)	(± dB)	(± dB)	
125 Hz	0.0	0.1	0.1	0.60	1.5	Pass
1000 Hz	0.0	0.0	0.0	0.60	1.0	Pass
4000 Hz	0.7	0.7	0.7	0.60	3.0	Pass
8000 Hz	1.4	1.4	1.5	0.70	3.0	Pass1

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of

เอกสารไม่ควบคุม

FSM-700-SLM-01 Rev.04 Issue date 5/6/24

Certificate No : 24-SLM-231
Request No : Req-2024-1450

5. Electrical signal test of frequency weightings, Weighting network response with relative to 1 kHz

UUC Setting	Deviation from various Frequency Weighting Response curve			UNCERTAINTY (± dB)	Acceptance Limit (± dB)	Result
	A (dB)	C (dB)	Z (dB)			
FAST / 37-139						
STD Setting						
63 Hz	-0.2	-0.1	-0.1	0.20	2.0	Pass
125 Hz	-0.1	0.0	-0.1		1.5	Pass
250 Hz	-0.1	0.0	-0.1		1.5	Pass
500 Hz	-0.1	0.0	-0.1		1.5	Pass
1000 Hz	0.0	0.0	-0.1		1.0	Pass
2000 Hz	0.0	0.0	0.0		2.0	Pass
4000 Hz	0.0	0.0	0.0		3.0	Pass
8000 Hz	-0.1	-0.1	0.0		5.0	Pass
16000 Hz	-0.1	-0.1	-0.1		+5, -INF	Pass

6. Frequency and time weightings at 1kHz

UUC Setting	STD REF	Measured		UNCERTAINTY (± dB)	Acceptance Limit (± dB)	Result
		UUC (dB)	ERR (dB)			
FAST / 37-139						
UUC Weighting						
A	114.00	114.0	0.0	0.20	0.20	Pass
C	114.00	114.0	0.0		0.20	Pass
Z	114.00	114.0	0.0		0.20	Pass

UUC Setting	STD REF	Measured		UNCERTAINTY (± dB)	Acceptance Limit (± dB)	Result
		UUC (dB)	ERR (dB)			
37-139 / A						
UUC Time Response						
Fast	114.00	114.0	0.0	0.20	0.10	Pass1
Slow	114.00	114.0	0.0		0.10	Pass1
Lsq	114.00	114.0	0.0		0.10	Pass1

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of

เอกสารไม่ควบคุม

FSM-700-SLM-01 Rev.04 Issue date 5/6/24

Certificate No : 24-SLM-231
Request No : Req-2024-1450

7. Long Term Stability

UUC Setting	Measured UUC (dB)	UNCERTAINTY (± dB)	Acceptance Limit (± dB)	Result
FAST / A / 37-139				
STD Setting				
Initial	114.0			
Final	114.0			
Deviated	0.0			
		0.10	0.30	Pass

8. Level linearity on the reference level range

UUC Setting	Anticipated REF	Deviation		UNCERTAINTY (± dB)	Acceptance Limit (± dB)	Result
		UUC (dB)	ERR (dB)			
FAST / A / 37-139						
STD dB	(dB)	(dB)	(dB)	(± dB)	(± dB)	
130.00	130	130.0	0.0	0.30	1.1	Pass
134.00	134	134.0	0.0		1.1	Pass
120.00	120	120.0	0.0		1.1	Pass
124.00	124	124.0	0.0		1.1	Pass
110.00	110	110.0	0.0		1.1	Pass
114.00	114	114.0	0.0		1.1	Pass
100.00	100	100.0	0.0		1.1	Pass
104.00	104	104.0	0.0		1.1	Pass
90.00	90	90.0	-0.1		1.1	Pass
94.00	94	93.9	-0.1		1.1	Pass
80.00	80	80.0	-0.1		1.1	Pass
84.00	84	83.9	-0.1		1.1	Pass
70.00	70	70.0	-0.1		1.1	Pass
74.00	74	73.9	-0.1		1.1	Pass
60.00	60	60.0	-0.1		1.1	Pass
64.00	64	63.9	-0.1		1.1	Pass
50.00	50	50.0	-0.1		1.1	Pass
54.00	54	53.9	-0.1		1.1	Pass
40.00	40	40.0	0.0		1.1	Pass
44.00	44	44.1	0.1		1.1	Pass
30.00	30	30.5	0.5		1.1	Pass

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of

เอกสารไม่ควบคุม

FSM-700-SLM-01 Rev.04 Issue date 5/6/24

Certificate No : 24-SLM-231
Request No : Req-2024-1450

9. Level linearity including the level range control

UUC Setting	STD REF	Measured		UNCERTAINTY (± dB)	Acceptance Limit (± dB)	Result
		UUC (dB)	ERR (dB)			
FAST / A						
UUC Range						
37-139	44.80	44.9	0.1	0.30	1.1	Pass
	114	114.0	0.0		1.1	Pass

10. Tone burst response

UUC Setting	STD Toneburst	Anticipated Ref	Measured		UNCERTAINTY (± dB)	Acceptance Limit (± dB)	Result
			UUC (dB)	ERR (dB)			
A / 37-139							
UUC Time Response	(ms)						
Fast	200	135.0	135.0	0.0	0.20	1.0	Pass
	2	118.0	117.9	-0.1		+1.0, -2.5	Pass
	0.25	109.0	108.6	-0.4		+1.5, -5.0	Pass
Slow	200	128.6	128.5	-0.1		1.0	Pass
	2	109.0	108.9	-0.1		+1.0, -5.0	Pass
	200	129.0	129.0	0.0		1.0	Pass
SEL	2	109.0	109.1	+0.1		+1.0, -2.5	Pass
	0.25	100.0	99.8	-0.2		+1.5, -5.0	Pass

11. Peak C Sound level

UUC Setting	Anticipated REF	Measured		UNCERTAINTY (± dB)	Acceptance Limit (± dB)	Result
FAST / C / 95-142		UUC (dB)	ERR (dB)			
STD Setting	(dB)	(dB)	(dB)	(± dB)	(± dB)	
Complete cycle	137.4	136.7	-0.70	0.20	3.0	Pass
Positive half cycle	136.4	136.2	-0.20		2.0	Pass
Negative half cycle	136.4	136.2	-0.20		2.0	Pass

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of

เอกสารไม่ควบคุม

FSM-700-SLM-01 Rev.04 Issue date 5/6/24

Certificate No : 24-SLM-231
Request No : Req-2024-1450

12. Overload indication

UUC Setting	Measured	UNCERTAINTY	Acceptance Limit	Result
FAST / A / 37-139	UUC	(± dB)	(± dB)	
STD Setting	(dB)			
Positive one-half cycle	143.7			
Negative one-half cycle	143.8			
Deviated	-0.1	0.20	1.5	Pass

13. High Level Stability

UUC Setting	Measured	UNCERTAINTY	Acceptance Limit	Result
FAST / A / 37-139	UUC	(± dB)	(± dB)	
STD Setting	(dB)			
Initial	138.0			
Final	138.0			
Deviated	0.0	0.10	0.30	Pass

Note :

Function	Maximum-permitted Uncertainty of measurement
1. Indication at the calibration check frequency	Not applicable
2. Self-generated noise, Microphone installed	Not applicable
3. Self-generated noise, Microphone replaced by the electrical input signal device	Not applicable
4. Acoustic signal test of frequency weightings at 10 Hz to 4 kHz	0.60 dB
4. Acoustic signal test of frequency weightings at >4 kHz to 10 kHz	0.70 dB
5. Electrical signal test of frequency weightings, Weighting network response with relative to 1 kHz	0.20 dB
6. Frequency and time weightings at 1kHz	0.20 dB
7. Long Term Stability	0.10 dB
8. Level linearity on the reference level range	0.30 dB
9. Level linearity including the level range control	0.30 dB
10. Tone burst response	0.30 dB
11. Peak C Second level	0.35 dB
12. Overload Indication	0.25 dB
13. High Level Stability	0.10 dB

* Acceptance limit and Maximum-permitted Uncertainty was IEC 61072-1:2013

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of

เอกสารไม่ควบคุม

FSM-708-SLM-01 Rev.04 Issue date 5/6/24

Certificate No : 24-SLM-231
Request No : Req-2024-1450

Decision Rule for Statements of Conformity


The standard decision rule employed for the statements of conformity to each calibration result will be applied using ILAC-G8:09:2019, Guidelines on the Reporting of Compliance with Specification as following Fig. and statements

Pass = The measurement result plus the expanded uncertainty with a 95% coverage probability were within the limit.

Pass¹ = The measurement result was within the limit. However, a portion of the expanded uncertainty of measurement at 95% exceeds the limit.

Fail¹ = The measurement result was out of the limit. However, a portion of the expanded uncertainty of measurement at 95% is within the limit.

Fail = The measurement result plus the expanded uncertainty with a 95% coverage probability, were outside the limit.

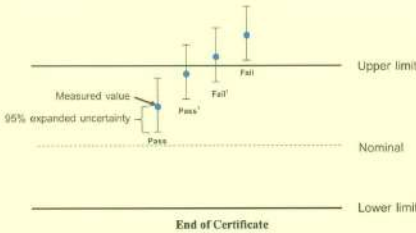

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of

เอกสารไม่ควบคุม

FSM-708-SLM-01 Rev.04 Issue date 5/6/24

Certificate of Calibration

Customer

Name : UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD. Certificate No : 24-SLM-232
Address : 81 Soi Udomak 41, Sukhumvit Road, Bangchak, Prakanong, Bangkok 10260 Request No : Req-2024-1451

Unit Under Calibration Details

Measurement item : Sound Level Meter Microphone Class : 2
Manufacturer : Larson Davis Microphone Model : 375H02
Model : LX72 Microphone S/N : 11793
Serial Number : 0605341 Pre-amplifier Model : PRMLxT2B
ID : UAEEFM.038/2563 Pre-amplifier S/N : 056133
Resolution : 0.1 dB Instrument Status : Used


Calibration Environment and Details

Temperature : 23 °C ± 2 °C
Humidity : 50 %RH ± 20 %RH
Barometric Pressure : 1013 hPa ± 10 hPa
Received Date : 1 July 2024
Calibrated Date : 10 July 2024
Calibration Procedure : In-house method CP-SLM-01 based on IEC 61072-3 : 2013 Electroacoustics - Sound level meters - Part 3: Periodic tests
Location of Calibration : Lab Acoustic

Reference Standard

Instrument	Brand	Model	SN	Due calibration	Traceability
Standard Microphone	GRAS	40AN	188273	30 August 2024	GRAS
Multifrequency Calibrator	Quest	Questcal	EFA000234	26 July 2024	TSI
Audio Generator	Svanick	Svan401	131	8 October 2024	WK Electric

Note
The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor k = 2, providing a level of confidence approximately 95 %.

Calibrated By : 
Mr. Noppadol Laungut
Service Calibration Engineer

Approved By : 
Mr. Paet Muthivorn
Calibration Engineer/Supervisor
Issue Date : 10 July 2024

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of

เอกสารไม่ควบคุม

FSM-708-SLM-01 Rev.04 Issue date 5/6/24

Certificate No : 24-SLM-232
Request No : Req-2024-1451

1. Indication at the calibration check frequency

UUC Setting	Nominal	Before Adjust		After Adjust		UNCERTAINTY (± dB)	Acceptance Limit (± dB)	Result
FAST / A / 37-139	Level	UUC	ERR	UUC	ERR			
Calibrator Setting	(dB)	(dB)	(dB)	(dB)	(dB)			
1000 Hz 114 dB	113.76	114.3	0.54	113.8	+0.04	0.20	0.30	Pass

Note : Absolute sensitivity was established by the use of Sound Calibrator Brand SVANTEK, Model SV 35A, SN. 58079

2. Self-generated noise, Microphone installed

UUC Setting	Measured	UNCERTAINTY
FAST / 37-139		
UUC Weighting	(dB)	(± dB)
A	29.7	0.10

3. Self-generated noise, Microphone replaced by the electrical input signal device

UUC Setting	Measured	UNCERTAINTY
FAST / 37-139		
UUC Weighting	(dB)	(± dB)
A	29.4	0.10
C	29.0	0.10
Z	33.0	0.10

4. Acoustic signal test of frequency weightings (Without Windscreen)

UUC Setting	Deviation from various Frequency Weighting Response curve			UNCERTAINTY (± dB)	Acceptance Limit (± dB)	Result
	A	C	Z			
	(dB)	(dB)	(dB)			
FAST / 37-139						
STD Setting	(dB)	(dB)	(dB)	(± dB)	(± dB)	
125 Hz	0.0	0.1	0.1	0.60	1.5	Pass
1000 Hz	0.0	0.0	0.0	0.60	1.0	Pass
4000 Hz	0.6	0.5	0.6	0.60	3.0	Pass
8000 Hz	1.0	0.9	1.0	0.70	5.0	Pass

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of

เอกสารไม่ควบคุม

FSM-708-SLM-01 Rev.04 Issue date 5/6/24



Certificate No : 24-SLM-232
Request No : Req-2024-1451

5. Electrical signal test of frequency weightings, Weighting network response with relative to 1 kHz

UUC Setting	Deviation from various Frequency			UNCERTAINTY	Acceptance Limit	Result
FAST / 37-139	Weighting Response curve					
STD Setting	A (dB)	C (dB)	Z (dB)	(± dB)	(± dB)	
63 Hz	-0.2	-0.1	-0.1	0.20	2.0	Pass
125 Hz	-0.1	0.0	-0.1		1.5	Pass
250 Hz	-0.1	0.0	-0.1		1.5	Pass
500 Hz	-0.1	0.0	-0.1		1.5	Pass
1000 Hz	0.0	0.0	-0.1		1.0	Pass
2000 Hz	0.0	0.0	0.0		2.0	Pass
4000 Hz	0.0	0.0	0.0		3.0	Pass
8000 Hz	-0.1	-0.1	0.0		5.0	Pass
16000 Hz	-0.1	-0.1	-0.1		+5, -INF	Pass

6. Frequency and time weightings at 1kHz

UUC Setting	STD	Measured		UNCERTAINTY (± dB)	Acceptance Limit (± dB)	Result
FAST / 37-139	REF	UUC	ERR			
UUC Weighting	(dB)	(dB)	(dB)			
A	114.00	114.0	0.0	0.20	0.20	Pass
C	114.00	114.0	0.0		0.20	Pass
Z	114.00	114.0	0.0		0.20	Pass

UUC Setting	STD	Measured		UNCERTAINTY (± dB)	Acceptance Limit (± dB)	Result
37-139 / A	REF	UUC	ERR			
UUC Time Response	(dB)	(dB)	(dB)			
Fast	114.00	114.0	0.0	0.20	0.10	Pass
Slow	114.00	114.0	0.0		0.10	Pass
Log	114.00	114.0	0.0		0.10	Pass

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of **เอกสารไม่ควบคุม**
ISO 7800:SLM-01 Rev.04 Issue date: 5/6/24



Certificate No : 24-SLM-232
Request No : Req-2024-1451

9. Level linearity including the level range control

UUC Setting	STD	Measured		UNCERTAINTY (± dB)	Acceptance Limit (± dB)	Result
FAST / A	REF	UUC	ERR			
UUC Range	(dB)	(dB)	(dB)			
37-139	44.20	44.3	0.1	0.30	1.1	Pass
	114	114.0	0.0		1.1	Pass

10. Tone burst response

UUC Setting	STD	Anticipated	Measured		UNCERTAINTY (± dB)	Acceptance Limit (± dB)	Result
A / 37-139	Testburst	Ref	UUC	ERR			
UUC Time Response	(ms)	(dB)	(dB)	(dB)			
Fast	200	135.0	135.0	0.0	0.20	1.0	Pass
	2	118.0	117.8	-0.2		+1.0, -2.5	Pass
	0.25	109.0	108.5	-0.5		+1.5, -5.0	Pass
Slow	200	128.6	128.4	-0.2		1.0	Pass
	2	109.0	108.5	-0.2		+1.0, -5.0	Pass
	200	129.0	129.0	0.0		1.0	Pass
SEL	2	109.0	109.0	0.0		+1.0, -2.5	Pass
	0.25	100.0	99.7	-0.3		+1.5, -5.0	Pass

11. Peak C Sound level

UUC Setting	Anticipated	Measured		UNCERTAINTY (± dB)	Acceptance Limit (± dB)	Result
FAST / C / 95-142	REF	UUC	ERR			
STD Setting	(dB)	(dB)	(dB)			
Complete cycle	137.4	136.8	-0.60	0.20	3.0	Pass
Positive half cycle	136.4	136.2	-0.20		2.0	Pass
Negative half cycle	136.4	136.2	-0.20		2.0	Pass

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of **เอกสารไม่ควบคุม**
ISO 7800:SLM-01 Rev.04 Issue date: 5/6/24



Certificate No : 24-SLM-232
Request No : Req-2024-1451

7. Long Term Stability

UUC Setting	Measured	UNCERTAINTY (± dB)	Acceptance Limit (± dB)	Result
FAST / A / 37-139	UUC: (dB)			
STD Setting	(dB)			
Initial	114.0	0.10	0.30	Pass
Final	114.0			
Deviated	0.0			

8. Level linearity on the reference level range

UUC Setting	Anticipated	Deviation		UNCERTAINTY (± dB)	Acceptance Limit (± dB)	Result
FAST / A / 37-139	REF	UUC	ERR			
STD dB	(dB)	(dB)	(dB)			
139.00	139	139.0	0.0	0.50	1.1	Pass
134.00	134	134.0	0.0		1.1	Pass
129.00	129	129.0	0.0		1.1	Pass
124.00	124	124.0	0.0		1.1	Pass
119.00	119	119.0	0.0		1.1	Pass
114.00	114	114.0	0.0		1.1	Pass
109.00	109	109.0	0.0		1.1	Pass
104.00	104	104.0	0.0		1.1	Pass
99.00	99	99.0	0.0		1.1	Pass
94.00	94	94.0	0.0		1.1	Pass
89.00	89	89.0	0.0		1.1	Pass
84.00	84	84.0	0.0		1.1	Pass
79.00	79	79.0	0.0		1.1	Pass
74.00	74	74.0	0.0		1.1	Pass
69.00	69	69.0	0.0		1.1	Pass
64.00	64	64.0	0.0		1.1	Pass
59.00	59	59.0	0.0		1.1	Pass
54.00	54	54.0	0.0		1.1	Pass
49.00	49	49.1	0.1		1.1	Pass
44.00	44	44.2	0.2		1.1	Pass
39.00	39	39.5	0.5		1.1	Pass

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of **เอกสารไม่ควบคุม**
ISO 7800:SLM-01 Rev.04 Issue date: 5/6/24



Certificate No : 24-SLM-232
Request No : Req-2024-1451

12. Overload indication

UUC Setting	Measured	UNCERTAINTY (± dB)	Acceptance Limit (± dB)	Result
FAST / A / 37-139	UUC: (dB)			
STD Setting	(dB)			
Positive one-half cycle	143.2	0.20	1.5	Pass
Negative one-half cycle	143.3			
Deviated	-0.1			

13. High Level Stability

UUC Setting	Measured	UNCERTAINTY (± dB)	Acceptance Limit (± dB)	Result
FAST / A / 37-139	UUC: (dB)			
STD Setting	(dB)			
Initial	128.0	0.10	0.30	Pass
Final	128.0			
Deviated	0.0			

Note :

Function	Maximum-permitted Uncertainty of measurement
1. Indication at the calibration check frequency	Not applicable
2. Self-generated noise, Microphone installed	Not applicable
3. Self-generated noise, Microphone replaced by the electrical input signal device	Not applicable
4. Acoustic signal test of frequency weightings at 10 Hz to 4 kHz	0.60 dB
4. Acoustic signal test of frequency weightings at >4 kHz to 10 kHz	0.70 dB
5. Electrical signal test of frequency weightings, Weighting network response with relative to 1 kHz	0.20 dB
6. Frequency and time weightings at 1kHz	0.20 dB
7. Long Term Stability	0.10 dB
8. Level linearity on the reference level range	0.30 dB
9. Level linearity including the level range control	0.30 dB
10. Tone burst response	0.30 dB
11. Peak C Sound level	0.35 dB
12. Overload indication	0.25 dB
13. High Level Stability	0.10 dB

* Acceptance limit and Maximum-permitted Uncertainty was IEC 61672-1:2013

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of **เอกสารไม่ควบคุม**
ISO 7800:SLM-01 Rev.04 Issue date: 5/6/24

Certificate No : 24-SLM-232
Request No : Req-2024-1451

Decision Rule for Statements of Conformity


The standard decision rule employed for the statements of conformity to each calibration result will be applied using ILAC-G8:09/2009, Guidelines on the Reporting of Compliance with Specification as following Fig. and statements:

Pass = The measurement result plus the expanded uncertainty with a 95% coverage probability were within the limit.

Pass¹ = The measurement result was within the limit. However, a portion of the expanded uncertainty of measurement at 95% exceeds the limit.

Fail¹ = The measurement result was out of the limit. However, a portion of the expanded uncertainty of measurement at 95% is within the limit.

Fail = The measurement result plus the expanded uncertainty with a 95% coverage probability were outside the limit.

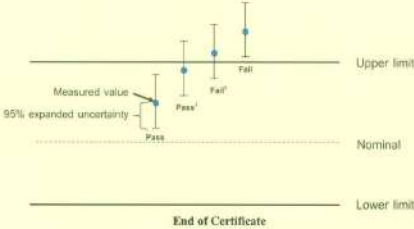

Certificate of Calibration

Customer : UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD. Certificate No : 24-SLM-235
Address : 81 Soi Udomrak 41, Sukhumvit Road, Bangchak, Prakanong, Bangkok Request No : Req-2024-1454
10260

Unit Under Calibration Details

Measurement Item : Sound Level Meter Microphone Class : 2
Manufacturer : Larson Davis Microphone Model : 375B02
Model : LX72 Microphone S/N : 11798
Serial Number : 0065346 Pre-amplifier Model : PRMLX72B
ID : UAEJFM.043/2563 Pre-amplifier S/N : 036138
Resolution : 0.1 dB Instrument Status : Used

Calibration Environment and Details


Temperature : 23 °C ± 2 °C
Humidity : 50 %RH ± 20 %RH
Barometric Pressure : 1013 hPa ± 10 hPa
Received Date : 1 July 2024
Calibrated Date : 10 July 2024
Calibration Procedure : In-house method CP-SLM-01 based on IEC 61672-3 :2013 Electroacoustics - Sound level meters - Part 3: Periodic tests
Location of Calibration : Lab Acoustic

Reference Standard

Instrument	Brand	Model	SN	Due calibration	Traceability
Standard Microphone	GRAS	40AN	188273	20 August 2024	GRAS
Multifrequency Calibrator	Quest	Quest-cal	EFA000234	26 July 2024	TSI
Audio Generator	SvanteK	Svan401	131	8 October 2024	W/K Electric

Note

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor k = 2, providing a level of confidence approximately 95 %.

Calibrated By : 
Mr. Nopadon Luangrat
Service Calibration Engineer

Approved By : 
Mr. Pachi Mathavorn
Calibration Engineer Supervisor
Issue Date : 10 July 2024

Certificate No : 24-SLM-235
Request No : Req-2024-1454

1. Indication at the calibration check frequency

UUC Setting FAST / A / 37-139	Nominal	Before Adjust		After Adjust		UNCERTAINTY (± dB)	Acceptance Limit (± dB)	Result
	Level (dB)	UUC (dB)	ERR (dB)	UUC (dB)	ERR (dB)			
1000 Hz 114 dB	113.76	115.3	1.54	113.8	+0.04	0.20	0.30	Pass

Note : Absolute sensitivity was established by the use of Sound Calibrator Brand SVANTER, Model SV 35A, SN. 30679

2. Self-generated noise, Microphone installed

UUC Setting FAST / 37-139	Measured (dB)	UNCERTAINTY (± dB)
A	31.4	0.10

3. Self-generated noise, Microphone replaced by the electrical input signal device

UUC Setting FAST / 37-139	Measured (dB)	UNCERTAINTY (± dB)
A	31.1	0.10
C	30.5	0.10
Z	35.0	0.10

4. Acoustic signal test of frequency weightings (Without Windscreen)

UUC Setting FAST / 37-139	Deviation from various Frequency Weighting Response curve			UNCERTAINTY (± dB)	Acceptance Limit (± dB)	Result
	A	C	Z			
STD Setting (dB)	(dB)	(dB)	(dB)	(± dB)	(± dB)	
125 Hz	0.0	0.1	0.1	0.60	1.5	Pass
1000 Hz	0.0	0.0	0.0	0.60	1.0	Pass
4000 Hz	1.1	1.1	1.1	0.60	3.0	Pass
8000 Hz	2.6	2.5	2.6	0.70	5.0	Pass

Certificate No : 24-SLM-235
Request No : Req-2024-1454

5. Electrical signal test of frequency weightings, Weighting network response with relative to 1 kHz

UUC Setting FAST / 37-139	Deviation from various Frequency Weighting Response curve			UNCERTAINTY (± dB)	Acceptance Limit (± dB)	Result
	A (dB)	C (dB)	Z (dB)			
STD Setting (dB)	(dB)	(dB)	(dB)	(± dB)	(± dB)	
63 Hz	-0.1	0.0	0.1	0.20	2.0	Pass
125 Hz	-0.1	0.0	0.0		1.5	Pass
250 Hz	-0.1	0.0	0.0		1.5	Pass
500 Hz	0.0	0.1	0.0		1.5	Pass
1000 Hz	0.0	0.0	0.0		1.0	Pass
2000 Hz	0.0	0.1	0.0		2.0	Pass
4000 Hz	0.0	-0.1	0.0		3.0	Pass
8000 Hz	-0.1	-0.1	0.0		5.0	Pass
16000 Hz	-0.1	-0.1	-0.1		+5, -INF	Pass

6. Frequency and time weightings at 1kHz

UUC Setting FAST / 37-139	STD REF	Measured		UNCERTAINTY (± dB)	Acceptance Limit (± dB)	Result
UUC Weighting (dB)	(dB)	UUC (dB)	ERR (dB)			
A	114.00	114.0	0.0	0.20	0.20	Pass
C	114.00	114.0	0.0		0.20	Pass
Z	114.00	114.0	0.0		0.20	Pass

UUC Setting 37-139 / A	STD REF	Measured		UNCERTAINTY (± dB)	Acceptance Limit (± dB)	Result
UUC Time Response (dB)	(dB)	UUC (dB)	ERR (dB)			
Fast	114.00	114.0	0.0	0.20	0.10	Pass
Slow	114.00	114.0	0.0		0.10	Pass
Lsq	114.00	114.0	0.0		0.10	Pass

7. Long Term Stability

UUC Setting	Measured	UNCERTAINTY	Acceptance	Result
FAST / A / 37-139	UUC	(± dB)	Limit (± dB)	
STD Setting	(dB)			
Initial	114.0			
Final	114.0			
Deviated	0.0	0.10	0.30	Pass

8. Level linearity on the reference level range

UUC Setting	Anticipated	Deviation		UNCERTAINTY	Acceptance	Result
FAST / A / 37-139	REF	UUC	ERR	(± dB)	Limit (± dB)	
STD dB	(dB)	(dB)	(dB)			
139.00	139	139.0	0.0			
134.00	134	134.0	0.0			
129.00	129	129.0	0.0			
124.00	124	124.0	0.0			
119.00	119	119.0	0.0			
114.00	114	114.0	0.0			
109.00	109	109.0	0.0			
104.00	104	104.0	0.0			
99.00	99	99.0	0.0			
94.00	94	94.0	0.0			
89.00	89	89.0	0.0			
84.00	84	84.0	0.0			
79.00	79	79.0	0.0			
74.00	74	74.0	0.0			
69.00	69	69.0	0.0			
64.00	64	64.0	0.0			
59.00	59	59.0	0.0			
54.00	54	54.0	0.0			
49.00	49	49.1	0.1			
44.00	44	44.2	0.2			
41.00	43	43.3	0.3			
42.00	42	42.3	0.3			
41.00	41	41.4	0.4			

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of **เอกสารไม่ควบคุม**
ISM-708-SLM-01 Rev.04 Issue date:5/8/24

12. Overload indication

UUC Setting	Measured	UNCERTAINTY	Acceptance	Result
FAST / A / 37-139	UUC	(± dB)	Limit (± dB)	
STD Setting	(dB)			
Positive one-half cycle	145.4			
Negative one-half cycle	145.3			
Deviated	0.1	0.20	1.5	Pass

13. High Level Stability

UUC Setting	Measured	UNCERTAINTY	Acceptance	Result
FAST / A / 37-139	UUC	(± dB)	Limit (± dB)	
STD Setting	(dB)			
Initial	138.0			
Final	138.0			
Deviated	0.0	0.10	0.30	Pass

Note :

Function	Maximum-permitted Uncertainty of measurement
1. Indication at the calibration check frequency	Not applicable
2. Self-generated noise, Microphone installed	Not applicable
3. Self-generated noise, Microphone replaced by the electrical input signal device	Not applicable
4. Acoustic signal test of frequency weightings at 10 Hz to 4 kHz	0.60 dB
4. Acoustic signal test of frequency weightings at >4 kHz to 10 kHz	0.70 dB
5. Electrical signal test of frequency weightings, Weighting network response with relative to 1 kHz	0.20 dB
6. Frequency and time weightings at 1kHz	0.20 dB
7. Long Term Stability	0.10 dB
8. Level linearity on the reference level range	0.30 dB
9. Level linearity including the level range control	0.30 dB
10. Tone burst response	0.30 dB
11. Peak C Sound level	0.35 dB
12. Overload indication	0.25 dB
13. High Level Stability	0.10 dB

* Acceptance limit and Maximum-permitted Uncertainty was IEC 61072-1:2013

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of **เอกสารไม่ควบคุม**
ISM-708-SLM-01 Rev.04 Issue date:5/8/24

9. Level linearity including the level range control

UUC Setting	STD	Measured		UNCERTAINTY	Acceptance	Result
FAST / A	REF	UUC	ERR	(± dB)	Limit (± dB)	
UUC Range	(dB)	(dB)	(dB)			
37-139	46.40	46.5	0.1			
	114	114.0	0.0	0.30	1.1	Pass

10. Tone burst response

UUC Setting	STD	Anticipated	Measured		UNCERTAINTY	Acceptance	Result
A / 37-139	Toneburst	Ref	UUC	ERR	(± dB)	Limit (± dB)	
UUC Time Response	(ms)	(dB)	(dB)	(dB)			
Fast	200	135.0	134.9	-0.1			
	2	118.0	117.8	-0.4			
	0.25	109.0	108.5	-0.5			
Slow	200	128.6	128.4	-0.2			
	2	109.0	108.8	-0.2			
	200	129.0	129.0	0.0			
SEL	2	109.0	108.8	-0.2			
	0.25	100.0	99.7	-0.3			

11. Peak C Sound level

UUC Setting	Anticipated	Measured		UNCERTAINTY	Acceptance	Result
FAST / C / 95-142	REF	UUC	ERR	(± dB)	Limit (± dB)	
STD Setting	(dB)	(dB)	(dB)			
Complete cycle	137.4	136.8	-0.60			
Positive half cycle	136.4	136.2	-0.20			
Negative half cycle	136.4	136.2	-0.20			

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of **เอกสารไม่ควบคุม**
ISM-708-SLM-01 Rev.04 Issue date:5/8/24

Decision Rule for Statements of Conformity


The standard decision rule employed for the statements of conformity to each calibration result will be applied using ILAC-G8:2019. Guidelines on the Reporting of Compliance with Specification as following Fig. and statements

Pass = The measurement result plus the expanded uncertainty with a 95% coverage probability were within the limit.

Pass¹ = The measurement result was within the limit. However, a portion of the expanded uncertainty of measurement at 95% exceeds the limit.

Fail¹ = The measurement result was out of the limit. However, a portion of the expanded uncertainty of measurement at 95% is within the limit.

Fail = The measurement result plus the expanded uncertainty with a 95% coverage probability were outside the limit.

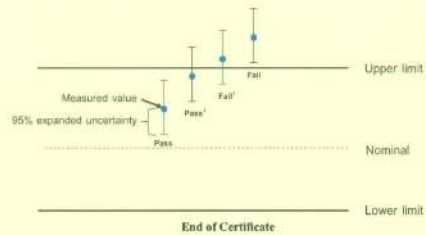

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of **เอกสารไม่ควบคุม**
ISM-708-SLM-01 Rev.04 Issue date:5/8/24



Certificate No.: CP20240292EA
Operation No.: CP2024070255

Certificate of Calibration

Equipment: Sound Level Meter

Manufacturer: Larson Davis (Meter), PCB (Microphone), PCB (Preamplifier)

Model/Type: LxT2 (Meter), 375B02 (Microphone), PRMLxT2B (Preamplifier)

Serial No.: 0005348 (Meter), 11800 (Microphone), 056140 (Preamplifier)

ID No.: UAE.EFM.045/2563

Customer: United Analyst and Engineering Consultant Co.,Ltd.


Address: 81 Soi Udomsuk 41, Sukhumvit Road, Bangchak
Phrakhanong, Bangkok 10260

Received Date: 25 July 2024

Calibrated Date: 6 - 7 August 2024

Issued Date: 7 August 2024

Calibrated by: Ms. Juntaporn Kunhakom

Approved by: 
(Mr. Sittichai Swaksuriyawong)
Group Manager

This report was prepared electronically using applicable electronic signature. Printing or copy of file are considered as a copy of the document.
The reported uncertainty of measurement was based on standard uncertainty multiplied by a coverage factor (k)
providing a level of confidence of approximately 95%. This certificate may not be reproduced other than in full except
with the prior written approval of the Electrical and Electronics Institute, Foundation for Industrial Development.

Page 1 of 6

เอกสารไม่ควบคุม

F-CAL-004 Ed.1



Certificate No.: CP20240292EA

Calibration Report

Equipment: Sound Level Meter

Manufacturer: Larson Davis (Meter), PCB (Microphone), PCB (Preamplifier)

Model/Type: LxT2 (Meter), 375B02 (Microphone), PRMLxT2B (Preamplifier)

Serial No.: 0005348 (Meter), 11800 (Microphone), 056140 (Preamplifier)

ID No.: UAE.EFM.045/2563

Ambient Temperature: (23 ± 2) °C

Relative Humidity: (50 ± 15) %

Pressure: (101.3 ± 1.5) kPa

Method of Calibration :-
IEC 61672-3:2013.

Condition of this result of calibration

1. Reference standards instrument :-

	Instrument	Model	Serial No.	Cert. No.	Due Date
1)	Standard microphone	4180	2787490	AA-1012-23	12 November 2024
2)	Arbitrary Function Generator	AFG2021	C010063	CK20240048EA	23 June 2025
3)	Programmable Attenuator	PA5	2755	EF-0040-23	1 October 2024
4)	6.5 Digit precision multimeter	8846A	9610014	CB20230200EA	15 November 2024
5)	Pressure humidity and Temperature Transmitter	PTU301	L3950483	CL1-P240023 CD20240142EA	24 March 2025 12 June 2025
6)	Pressure humidity and Temperature Transmitter	PTU301	L3950484	CL1-P240030 CD20240143EA	11 April 2025 12 June 2025
7)	Performance Audio Analyzer	U89038	MY56510003	CB20240035EB CK20230072EA	13 February 2025 13 September 2024

2. This result of calibration was found accurate as shown on date and place of calibration only.

3. This certification is traceable to the international system of unit maintained at :-

Reference standards instrument for Acoustic function

- National Institute of Metrology (Thailand)

Reference standards instrument for Electrical function

- National Institute of Metrology (Thailand)

- Electrical and Electronics Institute; NSC Accredited Calibration No.0119

Result of Calibration:-

Function : 1. Indication at the calibration check frequency

Reference Acoustic Signal (dB)	Measured value (dB)	Deviation (dB)	Acceptance limits (dB)
-	-	-	-

Page 2 of 6

F-CAL-005 Ed.1

เอกสารไม่ควบคุม



Certificate No.: CP20240292EA

Calibration Report

Function : 2. Self-generated Noise
2.1 Microphone Installed

Measured value (dB)
31.6

2.2 Microphone replaced by the electrical input signal device

Frequency Weighting	Measured value (dB)
A-weighting	31.5
C-weighting	31.6
Z-weighting	36.6

Function : 3. Acoustical signal tests of frequency weightings (Without Windscreen)

Meter free-field acoustic response at a level of 84 dB.

Frequency (Hz)	Deviation from various Frequency Weighting Response Curve			
	C-Weighting (dB)	A-Weighting (dB)	Z-Weighting (dB)	Acceptance limits (dB)
63	0.3	0.2	0.2	±1.5
125	-0.2	-0.2	-0.2	±1.0
8000	2.9	2.9	2.9	±5.0

Function : 4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various Frequency Weighting Response Curve			
	C-Weighting (dB)	A-Weighting (dB)	Z-Weighting (dB)	Acceptance limits (dB)
63	0.0	0.0	0.0	±2.0
125	0.0	0.0	0.0	±1.5
250	0.0	0.0	0.0	±1.5
500	0.1	0.0	0.0	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.1	0.0	0.0	±2.0
4000	0.0	0.0	0.0	±3.0
8000	0.0	0.0	0.1	±5.0

Function : 5. Frequency and time weighting at 1 kHz

5.1 Frequency weighting at 1 kHz

Frequency Weighting	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
C-weighting	94.0	0.0	±0.2
A-weighting	94.0	0.0	±0.2
Z-weighting	94.0	0.0	±0.2

เอกสารไม่ควบคุม

Page 3 of 6

F-CAL-005 Ed.1



Certificate No.: CP20240292EA

Calibration Report

5.2 Time weighting at 1 kHz

Time Weighting	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
Fast	94.0	0.0	±0.1
Slow	94.0	0.0	±0.1
LAeq	94.0	0.0	±0.1

Function : 6. Long-Term Stability

Long-term stability over 30 minutes, with steady 1 kHz signal at reference level.

Time Period to Apply Signal (min)	Reference SPL (dB)	Record SPL at Conclusion of Time Period (dB)	Deviated value (dB)	Acceptance limits (dB)
30	94.0	94.0	0.0	±0.3

Function : 7. Level Linearity on the reference level range

7.1 Level Linearity on the reference level range, Upper

Anticipated Value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
94.0	94.0	0.0	±1.1
99.0	99.0	0.0	±1.1
104.0	104.0	0.0	±1.1
109.0	109.0	0.0	±1.1
114.0	114.0	0.0	±1.1
119.0	119.0	0.0	±1.1
124.0	124.0	0.0	±1.1
129.0	129.0	0.0	±1.1
134.0	134.1	0.1	±1.1
139.0	139.1	0.1	±1.1
140.0	140.1	0.1	±1.1
141.0	141.1	0.1	±1.1
142.0	142.1	0.1	±1.1

เอกสารไม่ควบคุม

Page 4 of 6

F-CAL-005 Ed.1

Certificate No.: CP20240292EA

Calibration Report

7.2 Level Linearity on the reference level range, Lower

Anticipated Value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
94.0	94.0	0.0	±1.1
89.0	89.0	0.0	±1.1
84.0	84.0	0.0	±1.1
79.0	79.0	0.0	±1.1
74.0	74.0	0.0	±1.1
69.0	69.0	0.0	±1.1
64.0	64.0	0.0	±1.1
59.0	59.0	0.0	±1.1
54.0	54.0	0.0	±1.1
49.0	49.0	0.0	±1.1
44.0	44.1	0.1	±1.1
43.0	43.2	0.2	±1.1
42.0	42.3	0.3	±1.1
41.0	41.4	0.4	±1.1
40.0	40.5	0.5	±1.1

Function : 8. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
Fast	200	136.0	0.0	±1.0
	2	118.8	-0.2	+1.0 ; -2.5
	0.25	109.7	-0.3	+1.5 ; -5.0
Slow	200	129.5	-0.1	±1.0
	2	109.9	-0.1	+1.0 ; -5.0
	0.25	100.9	-0.1	+1.5 ; -5.0

Function : 9. Peak C sound level

Number of cycles in test signal	Anticipated Value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
Complete cycle	135.4	134.8	-0.6	±3.0
Positive half cycle	134.4	134.1	-0.3	±2.0
Negative half cycle	134.4	134.1	-0.3	±2.0

Function : 10. Overload indication

Measured value (dB)		Deviated value (dB)	Acceptance limits (dB)
Positive one-half cycle	Negative one-half cycle		
145.3	145.2	-0.1	±1.5

Page 5 of 6

F-CAL-005 Ed.1

เอกสารไม่ควบคุม

Certificate No.: CP20240292EA

Calibration Report

Function : 11. High-Level Stability

High-Level stability over 5 minutes, with steady 1 kHz signal, 1 dB below upper boundary.

Time Period to Apply Signal (min)	Reference SPL (dB)	Record SPL at Conclusion of Time Period (dB)	Deviated value (dB)	Acceptance limits (dB)
5	139.0	139.0	0.0	±0.3

Uncertainty of measurement

Function	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1) Indication at the calibration check frequency	0.30	Not applicable
2) Self-generated Noise	0.10	Not applicable
3) Acoustical signal tests of frequency weightings - Free-field sound pressure response level	0.30	0.60 (10Hz to 4kHz) 0.70 (>4kHz to 10kHz)
4) Electrical signal tests of frequency weightings	0.20	0.20
5) Frequency and time weighting at 1 kHz	0.20	0.20
6) Long-Term Stability	0.10	0.10
7) Level Linearity on the reference level range	0.30	0.30
8) Tone burst response	0.20	0.30
9) Peak C sound level	0.20	0.35
10) Overload indication	0.20	0.25
11) High-Level Stability	0.10	0.10

- Remarks:
1. Indication at the calibration check frequency can not measured because customer does not provide a sound calibrator.
 2. The acceptance limit is for the deviated value.
 3. Acceptance limits was IEC61672-3:2013 Class 2.
 4. The coverage factor $k = 2.00$

-- End of Report --

Page 6 of 6

F-CAL-005 Ed.1

เอกสารไม่ควบคุม



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL.0-2717-3000-29 FAX.0-2719-9484



Certificate of Calibration

Cert.No.: 24CH1153/1
Page.: 1 of 3

This Certificate was issued to replace to the Certificate No. 24CH1153

Equipment : pH Meter
Manufacturer : Horiba
Model : LAQUA-PH210
Serial No. : HA1G0008
ID No. : UAE.EFM.201/2564(EFM.pH.09/64)
Condition As-Received: Used Item
Received Date : 17 September 2024
Calibration Date : 18 September , 25 October 2024
Reference : 2409-0632WSC-1
Submitted by : United Analyst and Engineering Consultant Co.,Ltd.
3 Soi Udomsuk 41, Sukhumvit Road,
Bangchak, Phrakhanong, Bangkok 10260

Ambient Temperature : (25 ± 2.5) °C
Relative Humidity : (50 ± 15) %
Calibration Procedure : In - house method :
- CP-CH5 by direct measurement with DC voltage standard and direct measurement with certified reference material (CRM)
- CP-CH8 by comparison with temperature standard

Calibrated by : Warakorn Lemgatrakul**Approved by :** _____
Approved Signatory

() Unnopphol Harachai
() Ponpan Paipim
(✓) Saithip Meangmai

Issue Date : 28 October 2024

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written Approval of the head of Corporate Services 3: Equipment Calibration and Testing Services.

Cert.No.: 24CH1153/1
Page.: 2 of 3

Condition of this calibration result

1. Reference Standard Instrument

Instrument	Serial No.	ID No.	Cert. No.	Due Date
1) Document Process Calibrator	54030049	130RC116	24E2759	25 Aug 2025
2) Ref. Standard Thermometer	4982054	110RC044	24I757	14 July 2025

- This Certification is traceable to SI Through Technology Promotion Association (Thailand - Japan)

2. Certified Reference Materials :The measurement results are traceable to SI through Hach Lenge GmbH Ltd., Deutsche Akkreditierungsstelle, Accredited No.DRM-15184-01-00
:The measurement results are traceable to SI through CPA chem Ltd., ANSI-ASQ National Accreditation Board, Accredited No. AR-1835

Buffer Solution	Manufacturer	Lot No.	Exp. date
pH 4.006	Hach Lenge GmbH	C03146	23 Feb 2026
pH 7.000	Hach Lenge GmbH	C03020	13 Dec 2024
pH 9.997	CPA chem	970853	25 Apr 2025

3. This certificate is valid only to the item calibrated on date and place of calibration.

Calibration Results

Function : mV Measurement

Performing standard curve by Document Process Calibrator at pH (4,7)(7,10)

Unit Under Calibration	Nominal Value	Standard Voltage Input	Actual Reading		Uncertainty of Measurement	Coverage factor
	pH	mV	mV	pH	(±mV)	k
pH Meter S/N: HA1G0008	4.00	177.48	177.5	4.01	0.058	2.00
	7.00	0.00	0.0	7.02	0.058	2.00
	7.00	0.00	0.0	7.02	0.058	2.00
	10.00	-177.48	-177.5	10.01	0.058	2.00



Cert.No.: 24CH1153/1
Page.: 3 of 3

Calibration Results

Function : pH Measurement

Calibration Date : 18 September 2024

Performing three buffers standard curve by using buffer nominal pH (4,7)(7,10)

Unit Under Calibration	Standard pH Buffer Solution	Actual pH Reading	Actual mV Reading (mV)	Uncertainty of pH Measurement (\pm)	Coverage factor k
pH Electrode S/N.: -	4.006	4.01	168.7	0.0077	2.00
	7.000	6.99	-3.2	0.0084	2.00
	7.000	7.00	-3.4	0.0092	2.05
	9.997	10.01	-174.4	0.011	2.05

Function : Temperature Measurement

Calibration Date : 25 October 2024

(*) Without adjustment

This equipment was connected with Temperature Probe;

- Model : 9652

- Serial No. : -

Dimension of probe

- Length : 103 mm.

- Diameter : 16 mm.

- Immersion Depth : 90 mm.

Calibration Point ($^{\circ}\text{C}$)	Standard Temperature ($^{\circ}\text{C}$)	UUC* Reading ($^{\circ}\text{C}$)	Error ($^{\circ}\text{C}$)	Uncertainty of measurement (\pm $^{\circ}\text{C}$)	Coverage factor k
20.0	20.001	20.0	-0.001	0.13	2.00
25.0	25.005	25.0	-0.005	0.13	2.00
45.0	45.004	44.9	-0.104	0.13	2.00

Remark : - UUC* = Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k , providing a level of confidence of approximately 95 %.

-000-



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3 : EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000 FAX. 0-2719-9484

Certificate of Testing

Cert.No.: 24TW200
Page.: 1 of 2

Equipment : DO Meter
Manufacturer : Horiba
Model : LAQUA-DO210
Serial No. : HE1D0010
ID No. : UAE.EFM.208/2564(EFM.DO.10/64)
Received Date : 17 September 2024
Test Date : 18 September 2024
Reference : 2409-0633WSC-1
Submitted by : United Analyst and Engineering Consultant Co.,Ltd.
3 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Laboratory Condition : Temperature (25 ± 5) $^{\circ}\text{C}$
Humidity (50 ± 20) %
Test Procedure : In - house method : CP-CH9
by Comparison Technique with Azide Modification Method
Tested by : Walalak Sirithean
Approved by :
Approved Signatory
() Unnopphol Harachai
() Ponpan Paipim
(✓) Saithip Meangmai
Issue Date : 18 September 2024



Cert.No.: 24TW200
Page.: 2 of 2

Condition of this result of calibration

1. Reference Standard Instruments :

This certification is traceable to the International System of Unit through the reference standards Laboratory of Industrial Calibration Center, Technology Promotion Association (Thailand-Japan).

Instruments	Serial No.	ID No.	Certificate No.	Due Date
1. Burette	-	130BU10	23CG1172	22 Mar 2025
2. Balance	14233821	110RC001	24MM131	04 July 2025

2. Standard Material :-

Material	Manufacturer	Lot.No.	Assay
Sodium Thiosulfate 5-Hydrate AR	KEMAUS	2203162447	99.6%

Result : Dissolved Oxygen Meter Adjustment With Air 100 %
Dissolved Oxygen Probe No.: 9K1B0023

Titration Method (Azide Modification Method) (mg/L)	DO Meter Reading (mg/L)	Standard Deviation (mg/L)
8.18	8.19	0.0055

This report was certified only for the instrument we tested. It is allowable to use for study Intend to use for advertising and referral purpose is prohibited. This report may not be reproduced other in full, without written approval of the laboratory

-000-



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3 : EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000-29 FAX. 0-2719-9484



Certificate of Calibration

Cert. No.: 24LM150
Page.: 1 of 2

Equipment : DO Meter with Sensor
Manufacturer : Horiba
Model : LAQUA-DO210
Serial No. : HE1D0010
ID No. : UAE.EFM.208/2564(EFM.DO.10/64)
Submitted by : United Analyst and Engineering Consultant Co.,Ltd.
3 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Location : TPA On Site Calibration Laboratory
Received Order : 17 September 2024
Calibrated Date : 18 September 2024
Ambient Temperature : (26 ± 10) $^{\circ}\text{C}$
Relative Humidity : (50 ± 30) %
AC Line Voltage : (220 ± 22) V
Calibrated by : Warakorn Lernagatrakul
Approved by :
Approved Signatory
() Ponpan Paipim
() Suwit Injai
(✓) Kunchit Promprat
Issue Date : 21 September 2024

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

เอกสารไม่ควบคุม

เอกสารไม่ควบคุม



Equipment : DO Meter with Sensor
Condition As-Received : Used Item
Reference : 2409-0633WSC-2
Cert. No.: 24LM150
Page.: 2 of 2

Procedure Used :-
Calibration were conducted using in-house calibration procedure CP-OT01 according to comparison with Industrial Platinum Resistance Thermometer (IPRT) into Temperature Bath.
The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-
- | Instrument | Serial No. | Cert. No. | Traceable | Due Date |
|------------------------|------------|-----------|-----------|-------------|
| 1) Digital Thermometer | 2188080 | 231216 | TPA | 11 Oct 2024 |
2. This certificate is valid only to the item calibrated on date and place of calibration.
3. This certification is traceable to the International System of Unit.

Remark : TPA : Technology Promotion Association (Thailand - Japan)

Result of Calibration :- (*) Without Adjustment

Function : Temperature measurement.

This instrument was connected with temperature sensor, S/N.: 9K1B0023

Calibration Point (°C)	Immersion Depth (mm)	Standard Temperature (°C)	UUC* Reading (°C)	Error (°C)	Uncertainty (± °C)	Coverage Factor k
25.0	80	25.002	25.0	-0.002	0.16	2.00
30.0	80	30.003	30.0	-0.003	0.16	2.00
35.0	80	35.004	35.0	-0.004	0.16	2.00

UUC* : Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

เอกสารไม่ควบคุม

ภาคผนวก ช

หนังสืออนุญาตขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน



ที่ อก ๐๓๑๐(๑)/ ๑ ๙ ๑

กรมโรงงานอุตสาหกรรม
ถนนพระรามที่ ๖ แขวงทุ่งพญาไท
เขตราชเทวี กรุงเทพฯ ๑๐๔๐๐

๒ ๙ กุมภาพันธ์ ๒๕๖๔

เรื่อง ยกเลิกบุคลากรของห้องปฏิบัติการวิเคราะห์

เรียน กรรมการผู้จัดการ บริษัท ยูไนเต็ด แอมนาลิสต์ แอนด์ เอ็นจิเนียริง คอนซัลแตนท์ จำกัด

อ้างถึง คำขอขึ้นทะเบียน/ต่ออายุ/เปลี่ยนแปลงบุคลากร และชนิดสารเคมีของห้องปฏิบัติการวิเคราะห์เอกชน
ลงวันที่ ๑๘ กุมภาพันธ์ ๒๕๖๔

ตามคำขอที่อ้างถึง บริษัท ยูไนเต็ด แอมนาลิสต์ แอนด์ เอ็นจิเนียริง คอนซัลแตนท์ จำกัด
ห้องปฏิบัติการวิเคราะห์เอกชน เลขทะเบียน ๖-๑๔๔๕ สถานที่ตั้งเลขที่ ๓ ซอยอุดมสุข ๔๑ ถนนสุขุมวิท
แขวงบางจาก เขตพระโขนง กรุงเทพมหานคร ขอยกเลิกบุคลากร ความละเอียดแจ้งแล้ว นั้น

กรมโรงงานอุตสาหกรรมพิจารณาแล้ว ให้ยกเลิกเจ้าหน้าที่ห้องปฏิบัติการวิเคราะห์เอกชน
จำนวน ๓ ราย ได้แก่

- ๑) นายอภิสิทธิ์ ศรีคงแก้ว ทะเบียนเลขที่ ๖-๑๔๔๕-จ-๐๐๔๘
- ๒) นางสาวนันทิดา พรหมกวยถ่า ทะเบียนเลขที่ ๖-๑๔๔๕-จ-๐๑๗๐
- ๓) นายภูวดล เบื้องมา ทะเบียนเลขที่ ๖-๑๔๔๕-จ-๐๑๔๘

จึงเรียนมาเพื่อทราบ

ขอแสดงความนับถือ

(นายธีรวัฒน์ อิศรางกูร ณ อยุธยา)

รองอธิบดี ปฏิบัติราชการแทน

อธิบดีกรมโรงงานอุตสาหกรรม

กองวิจัยและเตือนภัยมลพิษโรงงาน

กลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษและทะเบียนห้องปฏิบัติการ

โทร. ๐ ๒๔๓๐ ๖๓๑๒ ต่อ ๒๑๐๓-๕

โทรสาร ๐ ๒๔๓๐ ๖๓๑๒ ต่อ ๒๑๔๙

ไปรษณีย์อิเล็กทรอนิกส์ saraban@diw.mail.go.th

ZAAE
UNITED ANALYST AND ENGINEERING
CONSULTANT COMPANY LIMITED

ธำมาญ์ทอง
ธำมาญ์ทอง



“อุตสาหกรรมก้าวไกล ประเทศไทยก้าวหน้า ร่วมกันพัฒนา อุตสาหกรรมสีเขียว”



ที่ อก ๐๓๑๐(๑)/ ๑ ๐ ๘ ๙

กรมโรงงานอุตสาหกรรม
ถนนพระรามที่ ๖ แขวงทุ่งพญาไท
เขตราชเทวี กรุงเทพฯ ๑๐๔๐๐

๐ ๗ กุมภาพันธ์ ๒๕๖๔

เรื่อง ต่ออายุหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน

เรียน กรรมการผู้จัดการ บริษัท ยูไนเต็ด แอมนาลิสต์ แอนด์ เอ็นจิเนียริง คอนซัลแตนท์ จำกัด

อ้างถึง คำขอขึ้นทะเบียน/ต่ออายุ/เปลี่ยนแปลงบุคลากร และชนิดสารเคมีของห้องปฏิบัติการวิเคราะห์เอกชน
ลงวันที่ ๓ ธันวาคม ๒๕๖๓

๑. รายชื่อผู้ควบคุมห้องปฏิบัติการวิเคราะห์เอกชน จำนวน ๔๐ ราย
๒. รายชื่อเจ้าหน้าที่ห้องปฏิบัติการวิเคราะห์เอกชน จำนวน ๑๔๑ ราย
๓. ขอบข่ายสารเคมีที่ได้รับขึ้นทะเบียนจากกรมโรงงานอุตสาหกรรม

ตามคำขอที่อ้างถึง บริษัท ยูไนเต็ด แอมนาลิสต์ แอนด์ เอ็นจิเนียริง คอนซัลแตนท์ จำกัด ขอต่ออายุ
หนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน เลขทะเบียน ๖-๑๔๔๕ สถานที่ตั้งเลขที่ ๓ ซอยอุดมสุข ๔๑
ถนนสุขุมวิท แขวงบางจาก เขตพระโขนง กรุงเทพมหานคร ต่อกรมโรงงานอุตสาหกรรม นั้น

กรมโรงงานอุตสาหกรรมพิจารณาแล้ว ให้บริษัท ยูไนเต็ด แอมนาลิสต์ แอนด์ เอ็นจิเนียริง
คอนซัลแตนท์ จำกัด ต่ออายุหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน โดยมีองค์ประกอบดังนี้

- ก. ผู้ควบคุมห้องปฏิบัติการวิเคราะห์เอกชน จำนวน ๔๐ ราย ตามสิ่งที่ส่งมาด้วย ๑
- ข. เจ้าหน้าที่ห้องปฏิบัติการวิเคราะห์เอกชน จำนวน ๑๔๑ ราย ตามสิ่งที่ส่งมาด้วย ๒
- ค. ขอบข่ายสารเคมีที่ได้รับขึ้นทะเบียนให้วิเคราะห์ในน้ำ/น้ำเสีย น้ำใต้ดิน อากาศเสีย
สิ่งปฏิกูลหรือวัสดุที่ไม่ใช้แล้ว และดิน ตามสิ่งที่ส่งมาด้วย ๓

หนังสือฉบับนี้จะหมดอายุในวันที่ ๒ กุมภาพันธ์ ๒๕๖๔ หากประสงค์จะต่ออายุหนังสือ
รับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน ให้ยื่นคำขอต่ออายุพร้อมเอกสารประกอบคำขอต่อกรมโรงงาน
อุตสาหกรรมภายใน ๖๐ วัน ก่อนวันสิ้นสุดของหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน

จึงเรียนมาเพื่อทราบ

ขอแสดงความนับถือ

(นายธีรวัฒน์ อิศรางกูร ณ อยุธยา)

รองอธิบดี ปฏิบัติราชการแทน

อธิบดีกรมโรงงานอุตสาหกรรม

ZAAE
UNITED ANALYST AND ENGINEERING
CONSULTANT COMPANY LIMITED

กองวิจัยและเตือนภัยมลพิษโรงงาน

กลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษและทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน

โทร. ๐ ๒๔๓๐ ๖๓๑๒ ต่อ ๒๑๐๓-๕

โทรสาร ๐ ๒๔๓๐ ๖๓๑๒ ต่อ ๒๑๔๙

ไปรษณีย์อิเล็กทรอนิกส์ saraban@diw.mail.go.th



“อุตสาหกรรมก้าวไกล ประเทศไทยก้าวหน้า ร่วมกันพัฒนา อุตสาหกรรมสีเขียว”



เอกสารแนบท้ายหนังสือต่ออายุบริษัททะเบียนห้องปฏิบัติการวิเคราะห์เอกชน

บริษัท ยูไนเต็ด แอนาไลติกส์ แอนด์ เอ็นจิเนียริง คอนซัลแตนท์ จำกัด เลขทะเบียน ๖-๑๔๕

ที่ ออ ๐๓๑๐(๑)/ ๑ ๐ ๘ ๙ ลงวันที่ ๐๗ กุมภาพันธ์ ๒๕๖๕

ก. ผู้ควบคุมห้องปฏิบัติการวิเคราะห์เอกชน จำนวน ๔๐ ราย

- ๑) นางสาวกชวรรณ ภักธีรกุล ทะเบียนเลขที่ ๖-๑๔๕-ค-๐๐๐๑
- ๒) นายณรงค์ ลิ้มพลี ทะเบียนเลขที่ ๖-๑๔๕-ค-๐๐๐๒
- ๓) นางสาวนันทา บุญไชย ทะเบียนเลขที่ ๖-๑๔๕-ค-๐๐๐๓
- ๔) นางปิยะพัชร สุทนต์วงษ์ ทะเบียนเลขที่ ๖-๑๔๕-ค-๐๐๐๔
- ๕) นางสาวเบญจวรรณ วิริโยทัย ทะเบียนเลขที่ ๖-๑๔๕-ค-๐๐๐๖
- ๖) นายพรรัตน์ วงศ์อนุรักษชัย ทะเบียนเลขที่ ๖-๑๔๕-ค-๐๐๐๗
- ๗) นางสาวฉวีวรรณ บุญลา ทะเบียนเลขที่ ๖-๑๔๕-ค-๐๐๐๘
- ๘) นายสุวิทย์ จอดนอก ทะเบียนเลขที่ ๖-๑๔๕-ค-๐๐๐๙
- ๙) นางสาวโชติภา สมบูรณ์ ทะเบียนเลขที่ ๖-๑๔๕-ค-๐๐๑๐
- ๑๐) นางสาวบุษกร เลิศกาญจนาศะ ทะเบียนเลขที่ ๖-๑๔๕-ค-๐๐๑๑
- ๑๑) นางสาววิไลลักษณ์ ศรีสุข ทะเบียนเลขที่ ๖-๑๔๕-ค-๐๐๑๒
- ๑๒) นายศิลา บรรจงใจรักษ์ ทะเบียนเลขที่ ๖-๑๔๕-ค-๐๐๑๔
- ๑๓) นายปฏิกรณ์ คณะนา ทะเบียนเลขที่ ๖-๑๔๕-ค-๐๐๑๕
- ๑๔) นายธีรวัฒน์ ขมิ้ม ทะเบียนเลขที่ ๖-๑๔๕-ค-๐๐๑๖
- ๑๕) นางสาวศิริพร ศรีประดิษฐ์ ทะเบียนเลขที่ ๖-๑๔๕-ค-๐๐๑๗
- ๑๖) นางสาวศิริกร รุ่ง ทะเบียนเลขที่ ๖-๑๔๕-ค-๐๐๑๘
- ๑๗) นางสาวพวรรณ อูราภัย ทะเบียนเลขที่ ๖-๑๔๕-ค-๐๐๑๙
- ๑๘) นายพงศ์ พานิชเลิศอำไพ ทะเบียนเลขที่ ๖-๑๔๕-ค-๐๐๒๐
- ๑๙) นายธีรวัฒน์ แดงสวัสดิ์ ทะเบียนเลขที่ ๖-๑๔๕-ค-๐๐๒๑
- ๒๐) นายเอกรัตน์ ปะคะมินทร์ ทะเบียนเลขที่ ๖-๑๔๕-ค-๐๐๒๒
- ๒๑) นางสาวนิศรัตน์ ศรีสกุลสิทธิ์โชค ทะเบียนเลขที่ ๖-๑๔๕-ค-๐๐๒๓
- ๒๒) นางสาวเจตจิรินทร์ ทำสะอาด ทะเบียนเลขที่ ๖-๑๔๕-ค-๐๐๒๔
- ๒๓) นางสาวสุวรรณ คงทอง ทะเบียนเลขที่ ๖-๑๔๕-ค-๐๐๒๕
- ๒๔) นางสาวกรรณ พัฒองขึ้น ทะเบียนเลขที่ ๖-๑๔๕-ค-๐๐๒๖
- ๒๕) นายวิรุฬห์ โมกแก้ว ทะเบียนเลขที่ ๖-๑๔๕-ค-๐๐๒๗
- ๒๖) นายวัชรพงษ์ เทพบุตร ทะเบียนเลขที่ ๖-๑๔๕-ค-๐๐๒๘
- ๒๗) นายอนุศาสน์ สายดี ทะเบียนเลขที่ ๖-๑๔๕-ค-๐๐๒๙
- ๒๘) นายกรวิทย์ เจริญศรีกุล ทะเบียนเลขที่ ๖-๑๔๕-ค-๐๐๓๐
- ๒๙) นายสุทธิระ อรุณจันทร์ ทะเบียนเลขที่ ๖-๑๔๕-ค-๐๐๓๑
- ๓๐) นางสาวทัศนีย์ อ่อนคำ ทะเบียนเลขที่ ๖-๑๔๕-ค-๐๐๓๒
- ๓๑) นายพรพรรณ กอนสิน ทะเบียนเลขที่ ๖-๑๔๕-ค-๐๐๓๔
- ๓๒) นายศุภณัฐ คุณอนกาญจน์ ทะเบียนเลขที่ ๖-๑๔๕-ค-๐๐๓๕
- ๓๓) นางสาวศิริภาพร หมอนแร่ ทะเบียนเลขที่ ๖-๑๔๕-ค-๐๐๓๗
- ๓๔) นางศิวาณัฐ ชินิล ทะเบียนเลขที่ ๖-๑๔๕-ค-๐๐๓๘
- ๓๕) นางสาวพรณิภา ธีระจินดาชล ทะเบียนเลขที่ ๖-๑๔๕-ค-๐๐๓๙

วันที่

๓๖) นายนาเคนทร์...

- ๓๖) นายนาเคนทร์ พันธุ์ชาติกุล ทะเบียนเลขที่ ๖-๑๔๕-ค-๐๐๔๐
- ๓๗) นายภาณุพงศ์ บุญพวง ทะเบียนเลขที่ ๖-๑๔๕-ค-๐๐๔๑
- ๓๘) นางสาวธรรมา แก้วชื่อนอก ทะเบียนเลขที่ ๖-๑๔๕-ค-๐๐๔๒
- ๓๙) นางสาวสริน ไชยเชษฐพัฒกุล ทะเบียนเลขที่ ๖-๑๔๕-ค-๐๐๔๓
- ๔๐) นามานิดา แย้มโย ทะเบียนเลขที่ ๖-๑๔๕-ค-๐๐๔๔

๓๖


เอกสารแนบท้ายหนังสือตอบรับชี้แจงทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน
บริษัท ยูไนเต็ด แอนาไลติกส์ แอนด์ เอ็นจิเนียริง คอนซัลแตนท์ จำกัด เลขทะเบียน ๖๔๕๕
ที่ อก ๐๓๑๐(๑)/ ๑ ๐ ๘ ๘ ลงวันที่ ๐๗ กุมภาพันธ์ ๒๕๖๔

ข. เจ้าหน้าที่ห้องปฏิบัติการวิเคราะห์เอกชน จำนวน ๑๔๑ ราย

๑) นายสุชนันต์ พันสิงห์	ทะเบียนเลขที่ ๖-๑๔๕๕-จ-๐๐๐๑
๒) นายพีรณัฐ เจริญผล	ทะเบียนเลขที่ ๖-๑๔๕๕-จ-๐๐๐๓
๓) นางสาวไอลักษณ์ เกษสุข	ทะเบียนเลขที่ ๖-๑๔๕๕-จ-๐๐๐๔
๔) นายสมชาติ อุหมั่น	ทะเบียนเลขที่ ๖-๑๔๕๕-จ-๐๐๐๕
๕) นางสาวปรมาภรณ์ ทองแก้ว	ทะเบียนเลขที่ ๖-๑๔๕๕-จ-๐๐๐๖
๖) นางสาวกัญญา สมพงษ์	ทะเบียนเลขที่ ๖-๑๔๕๕-จ-๐๐๐๗
๗) นางสาวรณิ สายบุญเรือน	ทะเบียนเลขที่ ๖-๑๔๕๕-จ-๐๐๑๐
๘) นายภกษณพงษ์ นามทิพย์	ทะเบียนเลขที่ ๖-๑๔๕๕-จ-๐๐๑๑
๙) นางสาวอาภากรณ์ อ่อนคง	ทะเบียนเลขที่ ๖-๑๔๕๕-จ-๐๐๑๒
๑๐) นายกิตติศักดิ์ ทรงจำรัส	ทะเบียนเลขที่ ๖-๑๔๕๕-จ-๐๐๑๓
๑๑) นางสาวอภิญญาพร บุญคง	ทะเบียนเลขที่ ๖-๑๔๕๕-จ-๐๐๑๔
๑๒) นางสาวพรพิมล แวนทอง	ทะเบียนเลขที่ ๖-๑๔๕๕-จ-๐๐๑๕
๑๓) นายอภิวิชญ์ ท่วงที	ทะเบียนเลขที่ ๖-๑๔๕๕-จ-๐๐๑๗
๑๔) นายมานิตย์ ปานโชติ	ทะเบียนเลขที่ ๖-๑๔๕๕-จ-๐๐๑๘
๑๕) นายศพร ธนะพุ่มพ์	ทะเบียนเลขที่ ๖-๑๔๕๕-จ-๐๐๑๙
๑๖) นางสาวกัญญาณี โยธา	ทะเบียนเลขที่ ๖-๑๔๕๕-จ-๐๐๒๐
๑๗) นางสาวเกตุ สุธิ	ทะเบียนเลขที่ ๖-๑๔๕๕-จ-๐๐๒๑
๑๘) นางสาวชนันญา อภิพัธปภา	ทะเบียนเลขที่ ๖-๑๔๕๕-จ-๐๐๒๒
๑๙) นายศิริพร จงคงเกียรติ	ทะเบียนเลขที่ ๖-๑๔๕๕-จ-๐๐๒๓
๒๐) นางสาวสุภาวดี อินทศรี	ทะเบียนเลขที่ ๖-๑๔๕๕-จ-๐๐๒๔
๒๑) นายพงษ์เทพ เหล่าจาง	ทะเบียนเลขที่ ๖-๑๔๕๕-จ-๐๐๒๕
๒๒) นายวิชญ์ พันทุกซ์	ทะเบียนเลขที่ ๖-๑๔๕๕-จ-๐๐๒๖
๒๓) นางสาวพัชริศา คดีพิศาล	ทะเบียนเลขที่ ๖-๑๔๕๕-จ-๐๐๒๗
๒๔) นางสาวเมกวิกา เสือคำจันทร์	ทะเบียนเลขที่ ๖-๑๔๕๕-จ-๐๐๒๘
๒๕) นายพีรพัฒน์ บุญศิริศิลป์	ทะเบียนเลขที่ ๖-๑๔๕๕-จ-๐๐๒๙
๒๖) นายพัชราลัย เลื่อนล่อง	ทะเบียนเลขที่ ๖-๑๔๕๕-จ-๐๐๓๐
๒๗) นายณัฐพงษ์ อนุธรรมรัตน์	ทะเบียนเลขที่ ๖-๑๔๕๕-จ-๐๐๓๑
๒๘) นายกันนิกร ระโศ	ทะเบียนเลขที่ ๖-๑๔๕๕-จ-๐๐๓๒
๒๙) นายปริญญา กลมเกลียว	ทะเบียนเลขที่ ๖-๑๔๕๕-จ-๐๐๓๓
๓๐) นายธีรวัจน มาตรโพธิ์ศรี	ทะเบียนเลขที่ ๖-๑๔๕๕-จ-๐๐๓๔
๓๑) นายบุญฤทธิพงษ์ ก้อนสิน	ทะเบียนเลขที่ ๖-๑๔๕๕-จ-๐๐๓๕
๓๒) นายพรพงษ์วุฒิ ไวกุล	ทะเบียนเลขที่ ๖-๑๔๕๕-จ-๐๐๓๖
๓๓) นายอชิระ แสงจันทร์	ทะเบียนเลขที่ ๖-๑๔๕๕-จ-๐๐๓๗
๓๔) ว่าที่ร้อยตรีรัฐพงศ์ เมื่องชัย	ทะเบียนเลขที่ ๖-๑๔๕๕-จ-๐๐๓๘
๓๕) นายอนันท์ เลิศประเสริฐ	ทะเบียนเลขที่ ๖-๑๔๕๕-จ-๐๐๓๙




๓๖) นางสาวนิภาพร จันทร์เขตต์	ทะเบียนเลขที่ ๖-๑๔๕๕-จ-๐๐๔๗
๓๗) นายรณภพ ภูตระกูลพัฒนา	ทะเบียนเลขที่ ๖-๑๔๕๕-จ-๐๐๔๘
๓๘) นายสมพงษ์ สกลไทย	ทะเบียนเลขที่ ๖-๑๔๕๕-จ-๐๐๔๙
๓๙) นายสุริยัน นิธิติตตพงศ์	ทะเบียนเลขที่ ๖-๑๔๕๕-จ-๐๐๕๐
๔๐) นายอัษฎาภรณ์ ยนต์ศิริ	ทะเบียนเลขที่ ๖-๑๔๕๕-จ-๐๐๕๑
๔๑) นายเอกวุฒิ แสนใจ	ทะเบียนเลขที่ ๖-๑๔๕๕-จ-๐๐๕๒
๔๒) นายสุชนันต์ บุญเลี้ยง	ทะเบียนเลขที่ ๖-๑๔๕๕-จ-๐๐๕๓
๔๓) นายธนเดช หวานแสนะ	ทะเบียนเลขที่ ๖-๑๔๕๕-จ-๐๐๕๔
๔๔) นายอภิสิทธิ์ ศรีคงแก้ว	ทะเบียนเลขที่ ๖-๑๔๕๕-จ-๐๐๕๕
๔๕) ว่าที่ร้อยตรีอุทัย แก้ววราภรณ์	ทะเบียนเลขที่ ๖-๑๔๕๕-จ-๐๐๕๖
๔๖) นางสาวนรินทร์ สานนท์	ทะเบียนเลขที่ ๖-๑๔๕๕-จ-๐๐๕๗
๔๗) นายศุภกร รินวงศ์	ทะเบียนเลขที่ ๖-๑๔๕๕-จ-๐๐๕๘
๔๘) นางสาวจินตสุภา เบ็ญศรี	ทะเบียนเลขที่ ๖-๑๔๕๕-จ-๐๐๕๙
๔๙) นางสาวนตรนภา กมลบุรณ์	ทะเบียนเลขที่ ๖-๑๔๕๕-จ-๐๐๖๐
๕๐) นางสาวอารียา ทรากรมย์	ทะเบียนเลขที่ ๖-๑๔๕๕-จ-๐๐๖๑
๕๑) นายจิรวัฒน์ สุขเกษม	ทะเบียนเลขที่ ๖-๑๔๕๕-จ-๐๐๖๒
๕๒) นายกิตติพงษ์ สอนชัยภูมิ	ทะเบียนเลขที่ ๖-๑๔๕๕-จ-๐๐๖๓
๕๓) นายจุฬพล สอนเพชร	ทะเบียนเลขที่ ๖-๑๔๕๕-จ-๐๐๖๔
๕๔) นางสาวพัชราภรณ์ แสงฟ้า	ทะเบียนเลขที่ ๖-๑๔๕๕-จ-๐๐๖๕
๕๕) นายรัตนชัย เหล่ามา	ทะเบียนเลขที่ ๖-๑๔๕๕-จ-๐๐๖๖
๕๖) นายอิทธิพงษ์ ศรีเดช	ทะเบียนเลขที่ ๖-๑๔๕๕-จ-๐๐๖๗
๕๗) นางสาวกรณิการ์ ลำลิทา	ทะเบียนเลขที่ ๖-๑๔๕๕-จ-๐๐๖๘
๕๘) นางสาวณัฐชา พรหมศิริ	ทะเบียนเลขที่ ๖-๑๔๕๕-จ-๐๐๖๙
๕๙) นายณกสิทธิ์ ศรีพิมพ์	ทะเบียนเลขที่ ๖-๑๔๕๕-จ-๐๐๗๐
๖๐) นางสาวลักขณา จันทร์สุข	ทะเบียนเลขที่ ๖-๑๔๕๕-จ-๐๐๗๑
๖๑) นายศักดิ์สินต์ นุ่มมี	ทะเบียนเลขที่ ๖-๑๔๕๕-จ-๐๐๗๒
๖๒) นายวรพงษ์ นนจันทร์	ทะเบียนเลขที่ ๖-๑๔๕๕-จ-๐๐๗๓
๖๓) นางสาวชนภา มาคะมาตร์	ทะเบียนเลขที่ ๖-๑๔๕๕-จ-๐๐๗๔
๖๔) นายณัฐชัย พรหมอารักษ์	ทะเบียนเลขที่ ๖-๑๔๕๕-จ-๐๐๗๕
๖๕) นายณรินทร์ พานแก้ว	ทะเบียนเลขที่ ๖-๑๔๕๕-จ-๐๐๗๖
๖๖) นายปรัชญาพล โสภ	ทะเบียนเลขที่ ๖-๑๔๕๕-จ-๐๐๗๗
๖๗) นายวัชรินทร์ แสนงาม	ทะเบียนเลขที่ ๖-๑๔๕๕-จ-๐๐๗๘
๖๘) นายอาทิตย์ อุดมผล	ทะเบียนเลขที่ ๖-๑๔๕๕-จ-๐๐๗๙
๖๙) นายอิทธิเดช ใจบุญ	ทะเบียนเลขที่ ๖-๑๔๕๕-จ-๐๐๘๐
๗๐) นายณิศาพร พงษ์ศิริ	ทะเบียนเลขที่ ๖-๑๔๕๕-จ-๐๐๘๑
๗๑) นายเสฏฐวุฒิ เอมกลิ่นบัว	ทะเบียนเลขที่ ๖-๑๔๕๕-จ-๐๐๘๒
๗๒) นางสาวนันทา หาญในเมือง	ทะเบียนเลขที่ ๖-๑๔๕๕-จ-๐๐๘๓
๗๓) นางสาวพิมพ์วรรณ สิมมา	ทะเบียนเลขที่ ๖-๑๔๕๕-จ-๐๐๘๔



๗๔) นายนิพนธ์วัฒน์ วงศ์คำ
๗๕) นายประพันธ์ยุทธ์ เฝือกนาง
๗๖) นางสาวคัมภีร์ ลาจิต
๗๗) นางสาวภาพร ชื่นมุกข์
๗๘) นางสาวบุญญา มอญงค์
๗๙) นายอมรพล อมรลักษณ์
๘๐) นางสาวศรีเพชร ทองขาว
๘๑) นางสาวนิชากร ศุภชาติไกรสร
๘๒) นางสาววิมลวรรณ คำตัน
๘๓) นายคุณานนท์ ฤทธาคณานนท์
๘๔) นายคุณรงค์ อ้อลอย
๘๕) นางสาวจิตรมาส ศรีวรรณ
๘๖) นายสุจิต โปชันเงิน
๘๗) นายธงนา ข่ายศรีภัก
๘๘) นายρχต เหมะจุลิน
๘๙) นายสรโชค หล้าไท
๙๐) นายชัย บัวสด
๙๑) นางสาวธัญญา ประสานศรี
๙๒) นายพดล น้อยนิยม
๙๓) นายศุภกร สนวนศรี
๙๔) นายคณพล ศิลานนท์
๙๕) นายไชยชัย พุ่มสว
๙๖) นายธีรวัฒน์ ธรรมสุวรรณ
๙๗) นายโพธิพงษ์ ชะขุนทด
๙๘) นางสาวณัฐกตา พลนิกรกิจ
๙๙) นางสาวงษ์ไพบร ทองบุรณ์
๑๐๐) นางสาวพริชิตา จรุงเนติยุทธ
๑๐๑) นางสาวเพ็ญพิชชา รอดทอง
๑๐๒) นางสาวณัฏฐา แสงสว่าง
๑๐๓) นายกิตติ ลืออาจ
๑๐๔) นายธนุพร คงศรี
๑๐๕) นางสาวสุภัทสร่า เอียนเงิน
๑๐๖) นางสาวพรรณทิพา อะโนนัม
๑๐๗) นายอนันต์ มุฑอ
๑๐๘) นางสาวพรพิมล ประชาพันธ์
๑๐๙) นายวิกรม บุญยเกียรติ
๑๑๐) นางสาวณัฐชา แก้วภาพ
๑๑๑) นายสิทธิพล พร้อมพອซ์นบุญ
๑๑๒) นางสาวนนท์ทิชา กลิ่นหนู

๑๑๓) นางสาวปิทยา...

ทะเบียนเลขที่ ๖-๑๔๕-จ-๐๑๑๑
ทะเบียนเลขที่ ๖-๑๔๕-จ-๐๑๑๒
ทะเบียนเลขที่ ๖-๑๔๕-จ-๐๑๑๓
ทะเบียนเลขที่ ๖-๑๔๕-จ-๐๑๑๔
ทะเบียนเลขที่ ๖-๑๔๕-จ-๐๑๑๕
ทะเบียนเลขที่ ๖-๑๔๕-จ-๐๑๑๖
ทะเบียนเลขที่ ๖-๑๔๕-จ-๐๑๑๗
ทะเบียนเลขที่ ๖-๑๔๕-จ-๐๑๑๘
ทะเบียนเลขที่ ๖-๑๔๕-จ-๐๑๑๙
ทะเบียนเลขที่ ๖-๑๔๕-จ-๐๑๒๐
ทะเบียนเลขที่ ๖-๑๔๕-จ-๐๑๒๑
ทะเบียนเลขที่ ๖-๑๔๕-จ-๐๑๒๒
ทะเบียนเลขที่ ๖-๑๔๕-จ-๐๑๒๓
ทะเบียนเลขที่ ๖-๑๔๕-จ-๐๑๒๔
ทะเบียนเลขที่ ๖-๑๔๕-จ-๐๑๒๕
ทะเบียนเลขที่ ๖-๑๔๕-จ-๐๑๒๖
ทะเบียนเลขที่ ๖-๑๔๕-จ-๐๑๒๗
ทะเบียนเลขที่ ๖-๑๔๕-จ-๐๑๒๘
ทะเบียนเลขที่ ๖-๑๔๕-จ-๐๑๒๙
ทะเบียนเลขที่ ๖-๑๔๕-จ-๐๑๓๐
ทะเบียนเลขที่ ๖-๑๔๕-จ-๐๑๓๑
ทะเบียนเลขที่ ๖-๑๔๕-จ-๐๑๓๒
ทะเบียนเลขที่ ๖-๑๔๕-จ-๐๑๓๓
ทะเบียนเลขที่ ๖-๑๔๕-จ-๐๑๓๔
ทะเบียนเลขที่ ๖-๑๔๕-จ-๐๑๓๕
ทะเบียนเลขที่ ๖-๑๔๕-จ-๐๑๓๖
ทะเบียนเลขที่ ๖-๑๔๕-จ-๐๑๓๗
ทะเบียนเลขที่ ๖-๑๔๕-จ-๐๑๓๘
ทะเบียนเลขที่ ๖-๑๔๕-จ-๐๑๓๙
ทะเบียนเลขที่ ๖-๑๔๕-จ-๐๑๔๐
ทะเบียนเลขที่ ๖-๑๔๕-จ-๐๑๔๑
ทะเบียนเลขที่ ๖-๑๔๕-จ-๐๑๔๒
ทะเบียนเลขที่ ๖-๑๔๕-จ-๐๑๔๓
ทะเบียนเลขที่ ๖-๑๔๕-จ-๐๑๔๔
ทะเบียนเลขที่ ๖-๑๔๕-จ-๐๑๔๕
ทะเบียนเลขที่ ๖-๑๔๕-จ-๐๑๔๖
ทะเบียนเลขที่ ๖-๑๔๕-จ-๐๑๔๗
ทะเบียนเลขที่ ๖-๑๔๕-จ-๐๑๔๘
ทะเบียนเลขที่ ๖-๑๔๕-จ-๐๑๔๙
ทะเบียนเลขที่ ๖-๑๔๕-จ-๐๑๕๐



๑๑๓) นางสาวปิทยา ขุจิตเชื้อ
๑๑๔) นางสาวลัดดาวัลย์ โพธิ์พันธ์
๑๑๕) นายอาทิตย์ ตาภา
๑๑๖) นางสาวบุญภาพร บุญอนนศรี
๑๑๗) นางสาวพัชรพรรณ จันธิบุตร
๑๑๘) นางสาวนฤกร ไถ่บ้านกาย
๑๑๙) นางสาวปวีณา แคนขมน
๑๒๐) นางสาวนันทิตา พรหมกวยถ้ำ
๑๒๑) นางสาวกมลชนก ปุ่มคำ
๑๒๒) นางสาวปาริฉัตร ทองใบ
๑๒๓) นายชัยวัฒน์ จันละคร
๑๒๔) นางสาวกัญญา สิงห์แก้ว
๑๒๕) นางสาวอรินา มะดีเยาะ
๑๒๖) นายฐาปกรณ์ อนุรา
๑๒๗) นางสาวชนันดา กิมาคม
๑๒๘) นายธนบดีนทร์ ยาเหลี่ยม
๑๒๙) นายวีระพงษ์ แสงท่าง
๑๓๐) นางสาวปิยะณัฐยา สำนภาพษ์
๑๓๑) นางสาวณัฏสร ศรีสถาน
๑๓๒) นางสาวจรรย์รัตน์ โสแทน
๑๓๓) นายธีรวัฒน์ พรหมลา
๑๓๔) นายณวิรัช ปลั่งกลาง
๑๓๕) นายณภัทร เตมียบุตร
๑๓๖) นางสาวจิตภา ฤชา
๑๓๗) นางสาวสุนตาทิพย์ สังข์ทอง
๑๓๘) นางสาวชรัส บาบุญ
๑๓๙) นายภูวดล เป็งมา
๑๔๐) ว่าที่ร้อยตรีณยุทธ ประทุมเขตต์
๑๔๑) นายอนุสร หล้าโรง



R/M

เอกสารแนบท้ายหนังสือต่ออายุรั้งขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน

บริษัท ยูไนเต็ด เอนเนอจี้ส์ แอนด์ เอ็นจิเนียริง คอนซัลแตนท์ จำกัด เลขทะเบียน ๖-๑๕๕

ที่ ออ ๐๓๑๐(๑) ๓ ๐ ๘ ๙ ลงวันที่ ๐๗ กุมภาพันธ์ ๒๕๖๕

ขอขยายสารมลพิษที่ได้รับขึ้นทะเบียนจากกรมโรงงานอุตสาหกรรม จำนวน ๓๕๓ รายการ

นับเปลี่ยน จำนวน 46 รายการ

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
1	Aldrin	Liquid-Liquid Extraction, Gas Chromatographic Method ⁽⁴⁾
2	Arsenic	1) Digestion, Hydride Generation/Atomic Absorption Spectrometric Method ⁽⁴⁾ 2) Digestion, Inductively Coupled Plasma Method ⁽⁴⁾
3	Barium	Digestion, Inductively Coupled Plasma Method ⁽⁴⁾
4	α-BHC	Liquid-Liquid Extraction, Gas Chromatographic Method ⁽⁴⁾
5	β-BHC	Liquid-Liquid Extraction, Gas Chromatographic Method ⁽⁴⁾
6	δ-BHC	Liquid-Liquid Extraction, Gas Chromatographic Method ⁽⁴⁾
7	γ-BHC	Liquid-Liquid Extraction, Gas Chromatographic Method ⁽⁴⁾
8	Biochemical Oxygen Demand	1) 5-Day BOD Test, Azide Modification Method ⁽⁴⁾ 2) 5-Day BOD Test, Membrane Electrode Method ⁽⁴⁾
9	Cadmium	1) Digestion, Direct Air-Acetylene Flame Method ⁽⁴⁾ 2) Digestion, Inductively Coupled Plasma Method ⁽⁴⁾
10	Chemical Oxygen Demand	1) Closed Reflux, Titrimetric Method ⁽⁴⁾ 2) Closed Reflux, Colorimetric Method ⁽⁴⁾ 3) Open Reflux, Titrimetric Method ⁽⁴⁾
11	Chlordane	Liquid-Liquid Extraction, Gas Chromatographic Method ⁽⁴⁾
12	Chromium	1) Digestion, Direct Air-Acetylene Flame Method ⁽⁴⁾ 2) Digestion, Inductively Coupled Plasma Method ⁽⁴⁾
13	Color	ADMI Weighted-Ordinate Spectrophotometric Method ⁽⁴⁾
14	Copper	1) Digestion, Direct Air-Acetylene Flame Method ⁽⁴⁾ 2) Digestion, Inductively Coupled Plasma Method ⁽⁴⁾
15	Cyanide	1) Distillation, Colorimetric Method ⁽⁴⁾ 2) Total Cyanide after Distillation, by Flow Injection Analysis Method ⁽⁴⁾
16	o,p'-DDT	Liquid-Liquid Extraction, Gas Chromatographic Method ⁽⁴⁾
17	4,4'-DDD	Liquid-Liquid Extraction, Gas Chromatographic Method ⁽⁴⁾
18	4,4'-DDE	Liquid-Liquid Extraction, Gas Chromatographic Method ⁽⁴⁾
19	4,4'-DDT	Liquid-Liquid Extraction, Gas Chromatographic Method ⁽⁴⁾
20	Dieldrin	Liquid-Liquid Extraction, Gas Chromatographic Method ⁽⁴⁾
21	Endosulfan I	Liquid-Liquid Extraction, Gas Chromatographic Method ⁽⁴⁾
22	Endosulfan II	Liquid-Liquid Extraction, Gas Chromatographic Method ⁽⁴⁾
23	Endosulfan sulfate	Liquid-Liquid Extraction, Gas Chromatographic Method ⁽⁴⁾
24	Endrin	Liquid-Liquid Extraction, Gas Chromatographic Method ⁽⁴⁾

25 Endrin aldehyde...

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
25	Endrin aldehyde	Liquid-Liquid Extraction, Gas Chromatographic Method ⁽⁴⁾
26	Formaldehyde	Distillation, Colorimetric Method ⁽²⁾
27	Free Chlorine	1) Iodometric Method ⁽⁴⁾ 2) DPD Ferrous Titrimetric Method ⁽⁴⁾
28	Heptachlor	Liquid-Liquid Extraction, Gas Chromatographic Method ⁽⁴⁾
29	Heptachlor Epoxide	Liquid-Liquid Extraction, Gas Chromatographic Method ⁽⁴⁾
30	Hexavalent Chromium	Colorimetric Method ⁽⁴⁾
31	Lead	1) Digestion, Direct Air-Acetylene Flame Method ⁽⁴⁾ 2) Digestion, Inductively Coupled Plasma Method ⁽⁴⁾
32	Manganese	1) Digestion, Direct Air-Acetylene Flame Method ⁽⁴⁾ 2) Digestion, Inductively Coupled Plasma Method ⁽⁴⁾
33	Mercury	Digestion, Cold-Vapor Atomic Absorption Spectrometric Method ⁽⁴⁾
34	Methoxychlor	Liquid-Liquid Extraction, Gas Chromatographic Method ⁽⁴⁾
35	Nickel	1) Digestion, Direct Air-Acetylene Flame Method ⁽⁴⁾ 2) Digestion, Inductively Coupled Plasma Method ⁽⁴⁾
36	Oil & Grease	1) Liquid-Liquid, Partition-Gravimetric Method ⁽⁴⁾ 2) Soxhlet Extraction Method ⁽⁴⁾
37	pH	Electrometric Method ⁽⁴⁾
38	Phenols	1) Distillation, Chloroform Extraction Method ⁽⁴⁾ 2) Distillation, Direct Photometric Method ⁽⁴⁾
39	Selenium	1) Digestion, Hydride Generation/Atomic Absorption Spectrometric Method ⁽⁴⁾ 2) Digestion, Inductively Coupled Plasma Method ⁽⁴⁾
40	Sulfide	1) Iodometric Method ⁽⁴⁾ 2) Methylene Blue Method ⁽⁴⁾
41	Temperature	Laboratory and Field Methods ⁽⁴⁾
42	Total Dissolved Solids	Dried at 180 °C ⁽⁴⁾
43	Total Kjeldahl Nitrogen	Semi-Micro-Kjeldahl Method ⁽⁴⁾
44	Total Suspended Solids	Dried from 103 to 105 °C ⁽⁴⁾
45	Trivalent Chromium	1) Digestion, Direct Air-Acetylene Flame Method; Colorimetric Method, Calculation ⁽⁴⁾ 2) Digestion, Inductively Coupled Plasma Method; Colorimetric Method, Calculation ⁽⁴⁾
46	Zinc	1) Digestion, Direct Air-Acetylene Flame Method ⁽⁴⁾ 2) Digestion, Inductively Coupled Plasma Method ⁽⁴⁾

น้ำได้ดื่ม...

แนบได้ค้น จำนวน 126 รายการ

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
1	Acenaphthene	1) Liquid-Liquid Extraction, Gas Chromatographic Method ⁽⁴⁾ 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾ Purge and Trap Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
2	Acetone	1) Liquid-Liquid Extraction, Gas Chromatographic Method ⁽⁴⁾
3	Aldrin	2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
4	Anthracene	1) Liquid-Liquid Extraction, Gas Chromatographic Method ⁽⁴⁾ 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾ Digestion, Inductively Coupled Plasma Method ⁽⁴⁾
5	Antimony	1) Digestion, Hydride Generation/Atomic Absorption Spectrometric Method ⁽⁴⁾
6	Arsenic	2) Digestion, Inductively Coupled Plasma Method ⁽⁴⁾
7	Atrazine	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
8	Barium	Digestion, Inductively Coupled Plasma Method ⁽⁴⁾
9	Benz(a)anthracene	1) Liquid-Liquid Extraction, Gas Chromatographic Method ⁽⁴⁾ 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
10	Benzene	2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾ Purge and Trap Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
11	Benzo(b)fluoranthene	1) Liquid-Liquid Extraction, Gas Chromatographic Method ⁽⁴⁾ 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
12	Benzo(k)fluoranthene	1) Liquid-Liquid Extraction, Gas Chromatographic Method ⁽⁴⁾ 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
13	Benzoic acid	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾

ฉบับที่ 1

14 Benzo(a)pyrene...

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
14	Benzo(a)pyrene	1) Liquid-Liquid Extraction, Gas Chromatographic Method ⁽⁴⁾ 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
15	Benzo(g,h,i)perylene	1) Liquid-Liquid Extraction, Gas Chromatographic Method ⁽⁴⁾ 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
16	Beryllium	Digestion, Inductively Coupled Plasma Method ⁽⁴⁾
17	Bis(2-chloroethyl)ether	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
18	Bis(2-ethylhexyl)phthalate	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
19	Bromodichloromethane	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
20	Bromoform	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
21	Butanol	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
22	Butyl benzyl phthalate	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
23	Cadmium	1) Digestion, Direct Air-Acetylene Flame Method ⁽⁴⁾ 2) Digestion, Electrothermal Atomic Absorption Spectrometric Method ⁽⁴⁾
24	Carbazole	3) Digestion, Inductively Coupled Plasma Method ⁽⁴⁾ Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
25	Carbon disulfide	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
26	Carbon tetrachloride	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
27	Chlordane	1) Liquid-Liquid Extraction, Gas Chromatographic Method ⁽⁴⁾ 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
28	p-Chloroaniline	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾

ฉบับที่ 1

29 Chlorobenzene...

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
29	Chlorobenzene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
30	Chlorodibromomethane	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
31	Chloroform	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
32	2-Chlorophenol	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
33	Chromium	1) Digestion, Direct Air-Acetylene Flame Method ⁽⁴⁾ 2) Digestion, Inductively Coupled Plasma Method ⁽⁴⁾
34	Chromium (III)	1) Digestion, Direct Air-Acetylene Flame Method; Colorimetric Method; Calculation ⁽⁴⁾ 2) Digestion, Inductively Coupled Plasma Method; Colorimetric Method; Calculation ⁽⁴⁾
35	Chromium (VI)	Colorimetric Method ⁽⁴⁾
36	Chrysene	1) Liquid-Liquid Extraction, Gas Chromatographic Method ⁽⁴⁾ 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
37	Cyanide	Distillation, Colorimetric Method ⁽⁴⁾
38	2,4-D	Liquid-Liquid Extraction, Gas Chromatographic Method ⁽⁴⁾
39	DDD	1) Liquid-Liquid Extraction, Gas Chromatographic Method ⁽⁴⁾ 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
40	DDE	1) Liquid-Liquid Extraction, Gas Chromatographic Method ⁽⁴⁾ 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
41	DDT	1) Liquid-Liquid Extraction, Gas Chromatographic Method ⁽⁴⁾ 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
42	Dibenz(a,h)anthracene	1) Liquid-Liquid Extraction, Gas Chromatographic Method ⁽⁴⁾ 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾

43 Di-n-butyl phthalate...

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
43	Di-n-butyl phthalate	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
44	1,2-Dichlorobenzene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
45	1,3-Dichlorobenzene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
46	1,4-Dichlorobenzene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
47	3,3'-Dichlorobenzidine	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
48	1,1-Dichloroethane	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
49	1,2-Dichloroethane	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
50	1,1-Dichloroethylene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
51	cis-1,2-Dichloroethylene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
52	trans-1,2-Dichloroethylene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
53	2,4-Dichlorophenol	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
54	1,2-Dichloropropane	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
55	1,3-Dichloropropane	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
56	1,3-Dichloropropene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
57	Dieldrin	1) Liquid-Liquid Extraction, Gas Chromatographic Method ⁽⁴⁾ 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
58	Diethyl phthalate	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
59	2,4-Dimethylphenol	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
60	2,4-Dinitrophenol	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾

61 2,4-Dinitrotoluene...

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
61	2,4-Dinitrotoluene	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
62	2,6-Dinitrotoluene	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
63	Di-n-Octyl phthalate	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
64	Endosulfan	1) Liquid-Liquid Extraction, Gas Chromatographic Method ⁽⁴⁾ 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
65	Endrin	1) Liquid-Liquid Extraction, Gas Chromatographic Method ⁽⁴⁾ 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
66	Ethylbenzene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
67	Fluoranthene	1) Liquid-Liquid Extraction, Gas Chromatographic Method ⁽⁴⁾ 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
68	Fluorene	1) Liquid-Liquid Extraction, Gas Chromatographic Method ⁽⁴⁾ 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
69	Heptachlor	1) Liquid-Liquid Extraction, Gas Chromatographic Method ⁽⁴⁾ 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
70	Heptachlor epoxide	1) Liquid-Liquid Extraction, Gas Chromatographic Method ⁽⁴⁾ 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
71	Hexachlorobenzene	1) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾ 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
72	Hexachloro-1,3-butadiene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
73	n-Hexane	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾

๗๗

74 α -HCH...

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
74	α -HCH	1) Liquid-Liquid Extraction, Gas Chromatographic Method ⁽⁴⁾ 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
75	β -HCH	1) Liquid-Liquid Extraction, Gas Chromatographic Method ⁽⁴⁾ 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
76	γ -HCH	1) Liquid-Liquid Extraction, Gas Chromatographic Method ⁽⁴⁾ 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
77	Hexachlorocyclopentadiene	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
78	Hexachloroethane	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
79	Indeno(1,2,3-cd)pyrene	1) Liquid-Liquid Extraction, Gas Chromatographic Method ⁽⁴⁾ 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
80	Isophorone	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
81	Lead	1) Digestion, Direct Air-Acetylene Flame Method ⁽⁴⁾ 2) Digestion, Electrothermal Atomic Absorption Spectrometric Method ⁽⁴⁾
82	Manganese	3) Digestion, Inductively Coupled Plasma Method ⁽⁴⁾ 1) Digestion, Direct Air-Acetylene Flame Method ⁽⁴⁾ 2) Digestion, Inductively Coupled Plasma Method ⁽⁴⁾
83	Mercury	Digestion, Cold-Vapor Atomic Absorption Spectrometric Method ⁽⁴⁾
84	Methanol	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
85	Methoxychlor	1) Liquid-Liquid Extraction, Gas Chromatographic Method ⁽⁴⁾ 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
86	Methyl bromide	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾

๗๘

87 Methylene chloride...

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
87	Methylene chloride	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
88	2-Methylphenol	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
89	2-Methylnaphthalene	1) Liquid-Liquid Extraction, Gas Chromatographic Method ⁽⁴⁾ 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
90	Methyl tert-butyl ether	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
91	Naphthalene	1) Liquid-Liquid Extraction, Gas Chromatographic Method ⁽⁴⁾ 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
92	Nickel	1) Digestion, Direct Air-Acetylene Flame Method ⁽⁴⁾ 2) Digestion, Inductively Coupled Plasma Method ⁽⁴⁾
93	Nitrobenzene	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
94	N-Nitrosodiphenylamine	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
95	N-Nitrosodi-n-propylamine	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
96	Polychlorinated Biphenyls	1) Liquid-Liquid Extraction, Gas Chromatographic Method ⁽⁴⁾ 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
- PCB 1016		
- PCB 1221		
- PCB 1232		
- PCB-1242		
- PCB-1248		
- PCB-1254		
- PCB-1260		
97	Pentachlorophenol	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
98	pH	Electrometric Method ⁽⁴⁾
99	Phenanthrene	1) Liquid-Liquid Extraction, Gas Chromatographic Method ⁽⁴⁾ 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾

จ
จก

100 Phenol...

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
100	Phenol	1) Distillation, Chloroform Extraction Method ⁽⁴⁾ 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
101	Pyrene	1) Liquid-Liquid Extraction, Gas Chromatographic Method ⁽⁴⁾ 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
102	Selenium	1) Digestion, Hydride Generation/Atomic Absorption Spectrometric Method ⁽⁴⁾ 2) Digestion, Inductively Coupled Plasma Method ⁽⁴⁾
103	Silver	Digestion, Inductively Coupled Plasma Method ⁽⁴⁾
104	Styrene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
105	1,1,2,2-Tetrachloroethane	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
106	Tetrachloroethylene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
107	Toluene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
108	Toxaphene	1) Liquid-Liquid Extraction, Gas Chromatographic Method ⁽⁴⁾ 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
109	TPH (C ₅ - C ₈)	1) Purge and Trap, Gas Chromatographic Method ⁽¹²²²⁾ 2) Purge and Trap, Gas Chromatographic/Mass spectrometric Method ⁽¹²²⁷⁾
110	TPH (C ₈ - C ₁₆)	Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method ⁽⁹²²⁾
111	TPH (C ₁₆ - C ₃₅)	Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method ⁽⁹²²⁾
112	1,2,4-Trichlorobenzene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
113	1,1,1-Trichloroethane	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
114	1,1,2-Trichloroethane	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
115	Trichloroethylene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾

จ
จก

116 2,4,5-Trichlorophenol...

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
116	2,4,5-Trichlorophenol	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
117	2,4,6-Trichlorophenol	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
118	1,3,5-Trimethylbenzene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
119	Vanadium	Digestion, Inductively Coupled Plasma Method ⁽⁴⁾
120	Vinyl acetate	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
121	Vinyl chloride	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
122	m-Xylene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
123	o-Xylene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
124	p-Xylene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
125	Xylene (Total)	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
126	Zinc	1) Digestion, Direct Air-Acetylene Flame Method ⁽⁴⁾ 2) Digestion, Inductively Coupled Plasma Method ⁽⁴⁾

อากาศเสีย (ปล่องระบาย) จำนวน 25 รายการ

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
1	Antimony	Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method ⁽⁵⁾
2	Arsenic	1) Isokinetic Sampling, Digestion, Hydride Generation/Atomic Absorption Spectrometric Method ⁽⁵⁾ 2) Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method ⁽⁵⁾
3	Cadmium	1) Isokinetic Sampling, Digestion, Direct Air-Acetylene Flame Method ⁽⁵⁾ 2) Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method ⁽⁵⁾
4	Carbon Monoxide	Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method ⁽⁵⁾
5	Chlorine	Instrumental Analyzer Method ⁽⁵⁾
6	Chromium	Isokinetic Sampling, Ion Chromatographic Method ⁽⁵⁾ 1) Isokinetic Sampling, Digestion, Direct Air-Acetylene Flame Method ⁽⁵⁾

Chromium (ต่อ)...

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
6	Chromium (ต่อ)	2) Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method ⁽⁵⁾
7	Cobalt	Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method ⁽⁵⁾
8	Copper	1) Isokinetic Sampling, Digestion, Direct Air-Acetylene Flame Method ⁽⁵⁾ 2) Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method ⁽⁵⁾
9	Cresol	Absorption Sampling, Gas Chromatographic Method ⁽⁵⁾
10	Dioxins/Furans	Isokinetic Sampling ⁽⁵⁾
11	Hydrogen Chloride	Isokinetic Sampling, Ion Chromatographic Method ⁽⁵⁾
12	Hydrogen Fluoride	Isokinetic Sampling, Ion Chromatographic Method ⁽⁵⁾
13	Hydrogen Sulfide	Absorption Sampling, Iodometric Method ⁽⁵⁾
14	Lead	1) Isokinetic Sampling, Digestion, Direct Air-Acetylene Flame Method ⁽⁵⁾ 2) Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method ⁽⁵⁾
15	Manganese	1) Isokinetic Sampling, Digestion, Direct Air-Acetylene Flame Method ⁽⁵⁾ 2) Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method ⁽⁵⁾
16	Mercury	Isokinetic Sampling, Digestion, Cold-Vapor Atomic Absorption Spectrometric Method ⁽⁵⁾
17	Nickel	1) Isokinetic Sampling, Digestion, Direct Air-Acetylene Flame Method ⁽⁵⁾ 2) Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method ⁽⁵⁾
18	Opacity	Ringelmann's Method ⁽¹⁾
19	Oxides of Nitrogen	1) Absorption Sampling, Phenoldisulfonic acid Method ⁽⁵⁾ 2) Instrumental Analyzer Method ⁽⁵⁾
20	Selenium	1) Isokinetic Sampling, Digestion, Hydride Generation/Atomic Absorption Spectrometric Method ⁽⁵⁾ 2) Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method ⁽⁵⁾
21	Sulfur Dioxide	1) Absorption Sampling, Barium-Thorin Titrimetric Method ⁽⁵⁾ 2) Instrumental Analyzer Method ⁽⁵⁾
22	Sulfuric Acid	Isokinetic Sampling, Barium-Thorin Titrimetric Method ⁽⁵⁾

23 Total Suspended Particulate...

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
23	Total Suspended Particulate	Isokinetic Sampling, Gravimetric Method ^[5]
24	Vanadium	Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method ^[5]
25	Xylene	1) Bag Sampling, Gas Chromatographic Method ^[5] 2) Adsorption Sampling, Gas Chromatographic Method ^[5]

สิ่งปฏิกูลหรือวัสดุที่ไม่ใช้แล้ว จำนวน 35 รายการ

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
1	Aldrin	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method ^[3,9,23] 2) Ultrasonic Extraction, Gas Chromatographic Method ^[10,23]
2	Antimony	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[3,6,14]
3	Arsenic	2) Digestion, Inductively Coupled Plasma Method ^[7,14] 1) Waste Extraction, Digestion, Hydride Generation/Atomic Absorption Spectrometric Method ^[3,6,16] 2) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[3,6,14] 3) Digestion, Hydride Generation/Atomic Absorption Spectrometric Method ^[7,16] 4) Digestion, Inductively Coupled Plasma Method ^[7,14]
4	Barium	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[3,6,14] 2) Digestion, Inductively Coupled Plasma Method ^[7,14]
5	Beryllium	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[3,6,14] 2) Digestion, Inductively Coupled Plasma Method ^[7,14]
6	Cadmium	1) Waste Extraction, Digestion, Flame Atomic Absorption Spectrometric Method ^[3,6,15] 2) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[3,6,14] 3) Digestion, Inductively Coupled Plasma Method ^[7,14]
7	Chlordane	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method ^[3,9,23] 2) Ultrasonic Extraction, Gas Chromatographic Method ^[10,23]

งาน

8 Chromium...

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
8	Chromium	1) Waste Extraction, Digestion, Flame Atomic Absorption Spectrometric Method ^[3,6,13] 2) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[3,6,14] 3) Digestion, Flame Atomic Absorption Spectrometric Method ^[7,15] 4) Digestion, Inductively Coupled Plasma Method ^[7,14]
9	Chromium (III)	1) Waste Extraction, Digestion, Flame Atomic Absorption Spectrometric Method; Waste Extraction, Colorimetric Method; Calculation ^[3,6,15,17] 2) Waste Extraction, Digestion, Inductively Coupled Plasma Method; Waste Extraction, Colorimetric Method; Calculation ^[3,6,14,17] 3) Digestion, Flame Atomic Absorption Spectrometric Method; Alkaline Digestion, Colorimetric Method; Calculation ^[7,8,15,17] 4) Digestion, Inductively Coupled Plasma Method; Alkaline Digestion, Colorimetric Method; Calculation ^[7,8,14,17]
10	Chromium (VI)	1) Waste Extraction, Colorimetric Method ^[3,17] 2) Alkaline Digestion, Colorimetric Method ^[8,17]
11	Cobalt	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[3,6,14]
12	Copper	2) Digestion, Inductively Coupled Plasma Method ^[7,14] 1) Waste Extraction, Digestion, Flame Atomic Absorption Spectrometric Method ^[3,6,15] 2) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[3,6,14]
13	2,4-D	3) Digestion, Flame Atomic Absorption Spectrometric Method ^[7,15] 4) Digestion, Inductively Coupled Plasma Method ^[7,14] 1) Waste Extraction, Gas Chromatographic Method ^[3,26] 2) Ultrasonic Extraction, Gas Chromatographic Method ^[10,23]
14	DDD	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method ^[3,9,23] 2) Ultrasonic Extraction, Gas Chromatographic Method ^[10,23]

งาน

15 DDE...

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
15	DDE	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method ^(3.9.23) 2) Ultrasonic Extraction, Gas Chromatographic Method ^(10.23)
16	DDT	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method ^(3.9.23) 2) Ultrasonic Extraction, Gas Chromatographic Method ^(10.23)
17	Dieldrin	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method ^(3.9.23) 2) Ultrasonic Extraction, Gas Chromatographic Method ^(10.23)
18	Endrin	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method ^(3.9.23) 2) Ultrasonic Extraction, Gas Chromatographic Method ^(10.23)
19	Heptachlor	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method ^(3.9.23) 2) Ultrasonic Extraction, Gas Chromatographic Method ^(10.23)
20	Lead	1) Waste Extraction, Digestion, Flame Atomic Absorption Spectrometric Method ^(3.6.15) 2) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^(3.6.14) 3) Digestion, Flame Atomic Absorption Spectrometric Method ^(7.15) 4) Digestion, Inductively Coupled Plasma Method ^(7.14)
21	Lindane	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method ^(3.9.23) 2) Ultrasonic Extraction, Gas Chromatographic Method ^(10.23)
22	Mercury	1) Waste Extraction, Digestion, Cold-Vapor Atomic Absorption Spectrometric Method ^(3.19) 2) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^(3.6.14) 3) Digestion, Cold-Vapor Atomic Absorption Spectrometric Method ⁽¹⁹⁾ 4) Digestion, Inductively Coupled Plasma Method ^(7.14)

Signature: *[Signature]*
ตำแหน่ง: *[ตำแหน่ง]*
UNITED ANALYST AND ENGINEERING CONSULTANT COMPANY LIMITED

๓๖

Mercury (ตะ)

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
22	Mercury (ตะ)	5) Thermal Decomposition Amalgamation and Atomic Absorption Spectrometric Method ⁽²⁰⁾ 1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method ^(3.9.23) 2) Ultrasonic Extraction, Gas Chromatographic Method ^(10.23)
23	Methoxychlor	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^(3.6.14) 2) Digestion, Inductively Coupled Plasma Method ^(7.14)
24	Molybdenum	1) Waste Extraction, Digestion, Flame Atomic Absorption Spectrometric Method ^(3.6.15) 2) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^(3.6.14)
25	Nickel	3) Digestion, Flame Atomic Absorption Spectrometric Method ^(7.15) 4) Digestion, Inductively Coupled Plasma Method ^(7.14)
26	Polychlorinated Biphenyls - Aroclor 1016 - Aroclor 1221 - Aroclor 1232 - Aroclor 1242 - Aroclor 1248 - Aroclor 1254 - Aroclor 1260 - 2-Chlorobiphenyl - 2,3-Dichlorobiphenyl - 2,2',5'-Trichlorobiphenyl - 2,4',5'-Trichlorobiphenyl - 2,2',3,5'-Tetrachlorobiphenyl - 2,2',5,5'-Tetrachlorobiphenyl - 2,3',4,4'-Tetrachlorobiphenyl - 2,2',3,4,5'-Pentachlorobiphenyl - 2,2',4,5,5'-Pentachlorobiphenyl - 2,3,3',4,6-Pentachlorobiphenyl	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method ^(3.9.24) 2) Ultrasonic Extraction, Gas Chromatographic Method ^(10.24)

Signature: *[Signature]*
ตำแหน่ง: *[ตำแหน่ง]*
UNITED ANALYST AND ENGINEERING CONSULTANT COMPANY LIMITED

๓๖

Polychlorinated Biphenyls (ตะ)

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
27	Polychlorinated Biphenyls(ตอ) - 2,2',3,4,4',5'- Hexachlorobiphenyl - 2,2',3,4,5,5'- Hexachlorobiphenyl - 2,2',3,5,5',6'- Hexachlorobiphenyl - 2,2',4,4',5,5'- Hexachlorobiphenyl - 2,2',3,3',4,4',5'- Heptachlorobiphenyl - 2,2',3,4,4',5,5'- Heptachlorobiphenyl - 2,2',3,4,4',5',6'- Heptachlorobiphenyl - 2,2',3,4',5,5',6'- Heptachlorobiphenyl - 2,2',3,3',4,4',5,5',6'- Nonachlorobiphenyl Pentachlorophenol	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^(3,9,28) 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^(10,28) Electrometric Method ^(31,32) 1) Waste Extraction, Digestion, Hydride Generation/Atomic Absorption Spectrometric Method ^(3,6,21) 2) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^(3,6,14) 3) Digestion, Hydride Generation/Atomic Absorption Spectrometric Method ^(7,21) 4) Digestion, Inductively Coupled Plasma Method ^(7,14) 1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^(3,6,14) 2) Digestion, Inductively Coupled Plasma Method ^(7,14) 1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^(7,14) 2) Digestion, Inductively Coupled Plasma Method ^(7,14)
28	pH	
29	Selenium	
30	Silver	
31	Thallium	

32 Toxaphene...

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
32	Toxaphene	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method ^(3,9,23) 2) Ultrasonic Extraction, Gas Chromatographic Method ^(10,23) 1) Waste Extraction, Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^(3,12,27) 2) Waste Extraction, Equilibrium Headspace, Gas Chromatographic/Mass Spectrometric Method ^(3,11,27) 3) Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^(13,27) 4) Equilibrium Headspace, Gas Chromatographic/Mass Spectrometric Method ^(11,27) 1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^(3,6,14) 2) Digestion, Inductively Coupled Plasma Method ^(7,14) 1) Waste Extraction, Digestion, Flame Atomic Absorption Spectrometric Method ^(3,6,15) 2) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^(3,6,14) 3) Digestion, Flame Atomic Absorption Spectrometric Method ^(7,15) 4) Digestion, Inductively Coupled Plasma Method ^(7,14)
33	Trichloroethylene	
34	Vanadium	
35	Zinc	

ดิน จำนวน 125 รายการ

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
1	Acenaphthene	1) Ultrasonic Extraction, Gas Chromatographic Method ^(10,25) 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^(10,28) Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^(13,27) 1) Ultrasonic Extraction, Gas Chromatographic Method ^(10,23) 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^(10,28) 1) Ultrasonic Extraction, Gas Chromatographic Method ^(10,25)
2	Acetone	
3	Aldrin	
4	Anthracene	1) Ultrasonic Extraction, Gas Chromatographic Method ^(10,25)

Anthracene (ตอ)...

ลำดับ	สารเคมี	วิธีวิเคราะห์
4	Anthracene (๓๑)	2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^(10,28)
5	Antimony	Digestion, Inductively Coupled Plasma Method ^(7,14)
6	Arsenic	1) Digestion, Hydride Generation/Atomic Absorption Spectrometric Method ^(7,16)
7	Atrazine	2) Digestion, Inductively Coupled Plasma Method ^(7,14)
8	Barium	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^(10,28)
9	Benz(a)anthracene	Digestion, Inductively Coupled Plasma Method ^(7,14)
10	Benzene	1) Ultrasonic Extraction, Gas Chromatographic Method ^(10,25)
11	Benzo(b)fluoranthene	2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^(10,28)
12	Benzo(k)fluoranthene	1) Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^(13,27)
13	Benzoic acid	2) Equilibrium Headspace, Gas Chromatographic/Mass Spectrometric Method ^(11,27)
14	Benzo(a)pyrene	1) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^(10,28)
15	Benzo(g,h,i)perylene	1) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^(10,28)
16	Beryllium	2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^(10,28)

17 Bis(2-chloroethyl)ether...

ลำดับ	สารเคมี	วิธีวิเคราะห์
17	Bis(2-chloroethyl)ether	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^(10,28)
18	Bis(2-ethylhexyl)phthalate	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^(10,28)
19	Bromodichloromethane	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^(13,27)
20	Bromoform	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^(13,27)
21	Butanol	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^(13,27)
22	Butyl benzyl phthalate	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^(10,28)
23	Cadmium	1) Digestion, Flame Atomic Absorption Spectrometric Method ^(7,15)
24	Carbazole	2) Digestion, Inductively Coupled Plasma Method ^(7,14)
25	Carbon disulfide	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^(10,28)
26	Carbon tetrachloride	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^(13,27)
27	Chlordane	1) Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^(13,27)
28	p-Chloroaniline	2) Equilibrium Headspace, Gas Chromatographic/Mass Spectrometric Method ^(11,27)
29	Chlorobenzene	1) Ultrasonic Extraction, Gas Chromatographic Method ^(10,23)
30	Chlorodibromomethane	2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^(10,28)
31	Chloroform	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^(10,28)
32	2-Chlorophenol	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^(13,27)

33 Chromium...

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
33	Chromium	1) Digestion, Flame Atomic Absorption Spectrometric Method ^(7,15) 2) Digestion, Inductively Coupled Plasma Method ^(7,16)
34	Chromium (III)	1) Digestion, Flame Atomic Absorption Spectrometric Method; Alkaline Digestion, Colorimetric Method; Calculation ^(7,8,15,17) 2) Digestion, Inductively Coupled Plasma Method; Alkaline Digestion, Colorimetric Method; Calculation ^(7,8,14,17) Alkaline Digestion, Colorimetric Method ^(8,17)
35	Chromium (VI)	1) Ultrasonic Extraction, Gas Chromatographic Method ^(10,25) 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^(10,28)
36	Chrysene	Extraction, Distillation, Colorimetric Method ^(29,30) Ultrasonic Extraction, Gas Chromatographic Method ⁽²⁶⁾
37	Cyanide	1) Ultrasonic Extraction, Gas Chromatographic Method ^(10,23) 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^(10,28)
38	2,4-D	1) Ultrasonic Extraction, Gas Chromatographic Method ^(10,23) 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^(10,28)
39	DDD	1) Ultrasonic Extraction, Gas Chromatographic Method ^(10,23) 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^(10,28)
40	DDE	1) Ultrasonic Extraction, Gas Chromatographic Method ^(10,23) 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^(10,28)
41	DDT	1) Ultrasonic Extraction, Gas Chromatographic Method ^(10,23) 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^(10,28)
42	Dibenz(a,h)anthracene	1) Ultrasonic Extraction, Gas Chromatographic Method ^(10,25) 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^(10,28)
43	Di-n-butyl phthalate	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^(10,28)
44	1,2-Dichlorobenzene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^(13,27)

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
45	1,3-Dichlorobenzene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^(13,27)
46	1,4-Dichlorobenzene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^(13,27)
47	3,3'-Dichlorobenzidine	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^(10,28)
48	1,1-Dichloroethane	1) Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^(13,27) 2) Equilibrium Headspace, Gas Chromatographic/Mass Spectrometric Method ^(11,27)
49	1,2-Dichloroethane	1) Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^(13,27) 2) Equilibrium Headspace, Gas Chromatographic/Mass Spectrometric Method ^(11,27)
50	1,1-Dichloroethylene	1) Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^(13,27) 2) Equilibrium Headspace, Gas Chromatographic/Mass Spectrometric Method ^(11,27)
51	cis-1,2-Dichloroethylene	1) Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^(13,27) 2) Equilibrium Headspace, Gas Chromatographic/Mass Spectrometric Method ^(11,27)
52	trans-1,2-Dichloroethylene	1) Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^(13,27) 2) Equilibrium Headspace, Gas Chromatographic/Mass Spectrometric Method ^(11,27)
53	2,4-Dichlorophenol	1) Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^(13,27) 2) Equilibrium Headspace, Gas Chromatographic/Mass Spectrometric Method ^(11,27)
54	1,2-Dichloropropane	1) Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^(13,27) 2) Equilibrium Headspace, Gas Chromatographic/Mass Spectrometric Method ^(11,27)
55	1,3-Dichloropropane	1) Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^(13,27) 2) Equilibrium Headspace, Gas Chromatographic/Mass Spectrometric Method ^(11,27)
56	1,3-Dichloropropene	1) Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^(13,27) 2) Equilibrium Headspace, Gas Chromatographic/Mass Spectrometric Method ^(11,27)
57	Dieldrin	1) Ultrasonic Extraction, Gas Chromatographic Method ^(10,23) 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^(10,28)

ลำดับ	สารมลพิษ	วิธีการวิเคราะห์
58	Diethyl phthalate	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^(10,28)
59	2,4-Dimethylphenol	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^(10,28)
60	2,4-Dinitrophenol	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^(10,28)
61	2,4-Dinitrotoluene	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^(10,28)
62	2,6-Dinitrotoluene	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^(10,28)
63	Di-n-Octyl phthalate	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^(10,28)
64	Endosulfan	1) Ultrasonic Extraction, Gas Chromatographic Method ^(10,23) 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^(10,28)
65	Endrin	1) Ultrasonic Extraction, Gas Chromatographic Method ^(10,23) 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^(10,28)
66	Ethylbenzene	1) Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^(13,27) 2) Equilibrium Headspace, Gas Chromatographic/Mass Spectrometric Method ^(11,27)
67	Fluoranthene	1) Ultrasonic Extraction, Gas Chromatographic Method ^(10,25) 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^(10,28)
68	Fluorene	1) Ultrasonic Extraction, Gas Chromatographic Method ^(10,25) 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^(10,28)
69	Heptachlor	1) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^(10,28) 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^(10,23)
70	Heptachlor epoxide	1) Ultrasonic Extraction, Gas Chromatographic Method ^(10,23)

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
70	Heptachlor epoxide (ต่อ)	2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^(10,28)
71	Hexachlorobenzene	1) Ultrasonic Extraction, Gas Chromatographic Method ^(10,23) 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^(10,28)
72	Hexachloro-1,3-butadiene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^(13,27)
73	n-Hexane	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^(13,27)
74	α -HCH	1) Ultrasonic Extraction, Gas Chromatographic Method ^(10,23) 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^(10,28)
75	β -HCH	1) Ultrasonic Extraction, Gas Chromatographic Method ^(10,23) 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^(10,28)
76	γ -HCH	1) Ultrasonic Extraction, Gas Chromatographic Method ^(10,23) 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^(10,28)
77	Hexachlorocyclopentadiene	1) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^(10,28) 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^(10,28)
78	Hexachloroethane	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^(10,28)
79	Indeno(1,2,3-cd)pyrene	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^(10,25) 1) Ultrasonic Extraction, Gas Chromatographic Method ^(10,25) 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^(10,28)
80	Isophorone	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^(10,28)
81	Lead	1) Digestion, Flame Atomic Absorption Spectrometric Method ^(7,15) 2) Digestion, Inductively Coupled Plasma Method ^(7,14)
82	Manganese	1) Digestion, Flame Atomic Absorption Spectrometric Method ^(7,15) 2) Digestion, Inductively Coupled Plasma Method ^(7,14)

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
83	Mercury	1) Digestion, Cold-Vapor Atomic Absorption Spectrometric Method ^[19] 2) Thermal Decomposition Amalgamation and Atomic Absorption Spectrometric Method ^[20] Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[13,27]
84	Methanol	1) Ultrasonic Extraction, Gas Chromatographic Method ^[10,23]
85	Methoxychlor	2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[10,28] Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[13,27]
86	Methyl bromide	1) Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[13,27]
87	Methylene chloride	2) Equilibrium Headspace, Gas Chromatographic/Mass Spectrometric Method ^[11,27]
88	2-Methylphenol	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[10,28]
89	2-Methylnaphthalene	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[10,28]
90	Methyl tert-butyl ether	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[13,27]
91	Naphthalene	1) Ultrasonic Extraction, Gas Chromatographic Method ^[10,25] 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[10,28]
92	Nickel	1) Digestion, Flame Atomic Absorption Spectrometric Method ^[7,15] 2) Digestion, Inductively Coupled Plasma Method ^[7,14]
93	Nitrobenzene	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[10,28]
94	N-Nitrosodiphenylamine	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[10,28]
95	N-Nitrosodi-n-propylamine	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[10,28]
96	Polychlorinated Biphenyls - Aroclor 1016	1) Ultrasonic Extraction, Gas Chromatographic Method ^[10,24]

ลำดับ	สารเคมี	วิธีวิเคราะห์
96	<p>Polychlorinated Biphenyls(ต่อไป)</p> <ul style="list-style-type: none"> - Aroclor 1221 - Aroclor 1232 - Aroclor 1242 - Aroclor 1248 - Aroclor 1254 - Aroclor 1260 <p>Polychlorinated Biphenyls</p> <ul style="list-style-type: none"> - 2-Chlorobiphenyl - 2,3-Dichlorobiphenyl - 2,2',5-Trichlorobiphenyl - 2,4',5-Trichlorobiphenyl - 2,2',3,5'-Tetrachlorobiphenyl - 2,2',5,5'-Tetrachlorobiphenyl - 2,3',4,4'-Tetrachlorobiphenyl - 2,2',3,4,5'- - Pentachlorobiphenyl - 2,2',4,5,5'- - Pentachlorobiphenyl - 2,3,3',4',6- - Pentachlorobiphenyl - 2,2',3,4,4',5'- - Hexachlorobiphenyl - 2,2',3,4,5,5'- - Hexachlorobiphenyl - 2,2',3,5,5',6- - Hexachlorobiphenyl - 2,2',4,4',5,5'- - Hexachlorobiphenyl - 2,2',3,3',4,4',5- - Heptachlorobiphenyl - 2,2',3,4,4',5,5'- - Heptachlorobiphenyl - 2,2',3,4,4',5',6- - Heptachlorobiphenyl - 2,2',3,4',5,5',6- - Heptachlorobiphenyl - 2,2',3,3',4,4',5,5',6- - Nonachlorobiphenyl 	<p>2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method^[10,28]</p> <p>Ultrasonic Extraction, Gas Chromatographic Method^[10,24]</p>

ลำดับ	สารเคมี	วิธีวิเคราะห์
97	Pentachlorophenol	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^(10,28)
98	Phenanthrene	1) Ultrasonic Extraction, Gas Chromatographic Method ^(10,29) 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^(10,28)
99	Phenol	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^(10,28)
100	Pyrene	1) Ultrasonic Extraction, Gas Chromatographic Method ^(10,29) 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^(10,28)
101	Selenium	1) Digestion, Hydride Generation/Atomic Absorption Spectrometric Method ^(7,21) 2) Digestion, Inductively Coupled Plasma Method ^(7,14)
102	Silver	Digestion, Inductively Coupled Plasma Method ^(7,14)
103	Styrene	1) Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^(13,27) 2) Equilibrium Headspace, Gas Chromatographic/Mass Spectrometric Method ^(11,27)
104	1,1,2,2-Tetrachloroethane	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^(13,27)
105	Tetrachloroethylene	1) Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^(13,27) 2) Equilibrium Headspace, Gas Chromatographic/Mass Spectrometric Method ^(11,27)
106	Toluene	1) Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^(13,27) 2) Equilibrium Headspace, Gas Chromatographic/Mass Spectrometric Method ^(11,27)
107	Toxaphene	Ultrasonic Extraction, Gas Chromatographic Method ^(10,23)
108	TPH (C ₅ -C ₈)	1) Purge and Trap, Gas Chromatographic Method ^(13,22) 2) Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^(10,22)
109	TPH (C ₅ -C ₁₆)	Ultrasonic Extraction, Gas Chromatographic Method ^(10,22)
110	TPH (C ₅ -C ₃₅)	Ultrasonic Extraction, Gas Chromatographic Method ^(10,22)

111 1,2,4-Trichlorobenzene...

ลำดับ	สารเคมี	วิธีวิเคราะห์
111	1,2,4-Trichlorobenzene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^(13,27)
112	1,1,1-Trichloroethane	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^(13,27)
113	1,1,2-Trichloroethane	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^(13,27)
114	Trichloroethylene	1) Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^(13,27) 2) Equilibrium Headspace, Gas Chromatographic/Mass Spectrometric Method ^(11,27)
115	2,4,5-Trichlorophenol	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^(10,28)
116	2,4,6-Trichlorophenol	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^(10,28)
117	1,3,5-Trimethylbenzene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^(13,27)
118	Vanadium	Digestion, Inductively Coupled Plasma Method ^(7,14)
119	Vinyl acetate	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^(13,27)
120	Vinyl chloride	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^(13,27)
121	m-Xylene	1) Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^(13,27) 2) Equilibrium Headspace, Gas Chromatographic/Mass Spectrometric Method ^(11,27)
122	o-Xylene	1) Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^(13,27) 2) Equilibrium Headspace, Gas Chromatographic/Mass Spectrometric Method ^(11,27)
123	p-Xylene	1) Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^(13,27) 2) Equilibrium Headspace, Gas Chromatographic/Mass Spectrometric Method ^(11,27)
124	Xylene (Total)	1) Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^(13,27) 2) Equilibrium Headspace, Gas Chromatographic/Mass Spectrometric Method ^(11,27)

125 Zinc...

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
125	Zinc	1) Digestion, Flame Atomic Absorption Spectrometric Method ^(7,15) 2) Digestion, Inductively Coupled Plasma Method ^(7,14)

เอกสารอ้างอิง

- กระทรวงอุตสาหกรรม. ประกาศกระทรวงอุตสาหกรรม, พ.ศ. 2549. เรื่อง กำหนดค่าปริมาณเขม่าควันที่เจือปนในอากาศที่ระบายออกจากปล่องของหม้อน้ำโรงสีข้าวที่เปลี่ยนแปลงเป็นเชื้อเพลิง. ราชกิจจานุเบกษา. 4 ธันวาคม 2549. เล่มที่ 123 ตอนพิเศษ 125/4.
- สมาคมวิศวกรรมสิ่งแวดล้อมแห่งประเทศไทย. คู่มือวิเคราะห์น้ำเสีย. พิมพ์ครั้งที่ 4. กรุงเทพฯ: เรือนแก้วการพิมพ์, 2547.
- กระทรวงอุตสาหกรรม. ประกาศกระทรวงอุตสาหกรรม, พ.ศ. 2566. เรื่อง การจัดการสิ่งปฏิกูลหรือวัสดุที่ไม่ใช้แล้ว. ราชกิจจานุเบกษา. 31 พฤษภาคม 2566. เล่มที่ 140 ตอนพิเศษ 126 ง.
- APHA, AWWA, WEF. Standard Methods for the Examination of Water and Wastewater. 24th ed. Washington, DC: APHA, 2023.
- United States Environmental Protection Agency. Standards of Performance for New Stationary Sources. 40 CFR 60. Appendix A, 2020.
- United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. SW-846, 2014.
- United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. Acid Digestion of Sediments, Sludges, and Soils. SW-846 Method 3050B, 1996.
- United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. Alkaline Digestion for Hexavalent Chromium. SW-846 Method 3060A, 1996.
- United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. Separatory Funnel Liquid-Liquid Extraction. SW-846 Method 3510C, 1996.
- United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. Ultrasonic Extraction. SW-846 Method 3550C, 2007.
- United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. Volatile Organic Compounds in Various Sample Matrices Using Equilibrium Headspace Analysis. SW-846 Method 5021A, 2014.
- United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. Purge and Trap for Aqueous Samples. SW-846 Method 5030C, 2003.
- United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. Closed System Purge and Trap and Extraction for Volatile Organics in Soil and Waste Sample. SW-846 Method 5035A, 2000.
- United States...

- United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. Inductively Coupled Plasma-Optical Emission Spectrometry. SW-846 Method 6010D, 2014.
- United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. Flame Atomic Absorption Spectrophotometry. SW-846 Method 7000B, 2007.
- United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. Arsenic (Atomic Absorption, Gaseous Hydride). SW-846 Method 7061A, 1992.
- United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. Chromium, Hexavalent (Colorimetric). SW-846 Method 7196A, 1992.
- United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. Mercury in Liquid Waste (Manual Cold Vapor Technique). SW-846 Method 7470A, 1994.
- United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. Mercury in Solid or Semisolid Waste (Manual Cold-Vapor Technique). SW-846 Method 7471B, 1998.
- United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. Mercury in Solids and Solutions by Thermal Decomposition, Amalgamation, and Atomic Absorption Spectrophotometry. SW-846 Method 7473, 2007.
- United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. Selenium (Atomic Absorption, Borohydride Reduction). SW-846 Method 7742, 1994.
- United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. Nonhalogenated Organics Using GC/FID. SW-846 Method 8015D, 2003.
- United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. Organochlorine Pesticides by Gas Chromatography. SW-846 Method 8081B, 2007.
- United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. Polychlorinated Biphenyls (PCBs) by Gas Chromatography. SW-846 Method 8082A, 2007.
- United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. Organochlorine Pesticides by Gas Chromatography. SW-846 Method 8081B, 2007.
- United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. Chlorinated Herbicides by GC Using Methylation or Pentafluorobenzoylation Derivatization. SW-846 Method 8151A, 1996.
- United States...


 RUK
 CONSULTANT COMPANY LIMITED

27. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. Volatile Organic Compounds by Gas Chromatography/ Mass Spectrometry. SW-846 Method 8260D, 2018.
28. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. Semivolatile Organic Compounds by Gas Chromatography/Mass Spectrometry. SW-846 Method 8270E, 2018.
29. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. Cyanide Extraction Procedure for Solids and Oils. SW-846 Method 9013A, 2014.
30. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. Cyanide in Waters and Extracts using Titrimetric and Manual Spectrophotometric Procedures. SW-846 Method 9014, 2014.
31. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. pH Electrometric Measurement. SW-846 Method 9040C, 2004.
32. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. Soil and Waste pH. SW-846 Method 9045D, 2004.

๓๑

