

ภาคผนวก จ
เอกสารสอบเทียบเครื่องมือวัด

List of Instruments Certification for Air & Noise Quality Analysis

No.	Instrument/Equipment	Parameter	Manufacturer	Model/Serial No.	Calibrator	Certification No.	Date of Calibration	Due date of Calibration	Remark
Ambient									
1	Orifice Transfer Standard Calibrator	Total Suspended Particulate (TSP) Particulate Matter < 10 µm (PM ₁₀)	Tisch Environmental, Inc.	TE-5025A 3383	Jiranatee Associates Co., Ltd.	COF-039-67	27 Sep 24	26 Sep 25	-
2	U-Tube Manometer	Total Suspended Particulate (TSP) Particulate Matter < 10 µm (PM ₁₀)	Dwyer	121-36-W/M -	Technology Promotion Association (Thailand-Japan)	25P112	19 Feb 25	18 Feb 26	-
3	Aneroid Barometer	Total Suspended Particulate (TSP) Particulate Matter < 10 µm (PM ₁₀)	Barigo, Germany	-	Technology Promotion Association (Thailand-Japan)	24P1856	4 Jun 24	3 Jun 25	-
4	Digital Thermo - Hygrometer	Total Suspended Particulate (TSP) Particulate Matter < 10 µm (PM ₁₀)	Digicon	TH-02 435031148	Technology Promotion Association (Thailand-Japan)	24H1487	15 Jul 24	14 Jul 25	-
5	Nitrogen Dioxide Analyzer	Nitrogen Dioxide	Thermo Scientific	42i CM19050148	UAE Consultant Co., Ltd.	20092024	20 Sep 24	19 Sep 25	-
6	Nitrogen Dioxide Analyzer	Nitrogen Dioxide	Thermo Scientific	42i CM19050149	UAE Consultant Co., Ltd.	17092024	17 Sep 24	16 Sep 25	-
7	Nitrogen Dioxide Analyzer	Nitrogen Dioxide	Thermo Scientific	42i CM22387036	UAE Consultant Co., Ltd.	04102024	4 Oct 24	3 Oct 25	-
8	Nitrogen Dioxide Analyzer	Nitrogen Dioxide	Thermo Scientific	42i CM22387037	UAE Consultant Co., Ltd.	04102024	4 Oct 24	3 Oct 25	-
9	Standard Gases (Mixture)	Nitrogen Dioxide	Airgas	EB0162121 2016PSIG	Airgas an Air Liquide company	E05NI91E15A0014	6 Jul 23	6 Jul 31	-
10	Sulphur Dioxide Analyzer	Sulphur Dioxide	Thermo Scientific	43i CM22387061	UAE Consultant Co., Ltd.	06092024	6 Sep 24	5 Sep 25	-
11	Sulphur Dioxide Analyzer	Sulphur Dioxide	Thermo Scientific	43i CM22387063	UAE Consultant Co., Ltd.	19062024	19 Jun 24	18 Jun 25	-
12	Sulphur Dioxide Analyzer	Sulphur Dioxide	Thermo Scientific	43i CM22387065	UAE Consultant Co., Ltd.	06092024	6 Sep 24	5 Sep 25	-
13	Sulphur Dioxide Analyzer	Sulphur Dioxide	Thermo Scientific	43i CM22387066	UAE Consultant Co., Ltd.	06092024	6 Sep 24	5 Sep 25	-
14	Standard Gases (Mixture)	Sulphur Dioxide	Airgas	EB0162121 2016PSIG	Airgas an Air Liquide company	E05NI91E15A0014	6 Jul 23	6 Jul 31	-

List of Instruments Certification for Air & Noise Quality Analysis

No.	Instrument/Equipment	Parameter	Manufacturer	Model/Serial No.	Calibrator	Certification No.	Date of Calibration	Due date of Calibration	Remark
Ambient									
15	Carbon Monoxide Analyzer	Carbon Monoxide	Thermo	48i 1200906880	UAE Consultant Co.,Ltd.	09092024	9 Sep 24	8 Sep 25	-
16	Carbon Monoxide Analyzer	Carbon Monoxide	Thermo	48i 1201497730	UAE Consultant Co.,Ltd.	09092024	9 Sep 24	8 Sep 25	-
17	Carbon Monoxide Analyzer	Carbon Monoxide	Thermo	48i 1201497732	UAE Consultant Co.,Ltd.	09092024	9 Sep 24	8 Sep 25	-
18	Carbon Monoxide Analyzer	Carbon Monoxide	Thermo	48i 1201497733	UAE Consultant Co.,Ltd.	14062024	14 Jun 24	13 Jun 25	-
19	Standard Gases (Mixture)	Carbon Monoxide	Airgas	EB0162121 2016PSIG	Airgas an Air Liquide company	E05NI91E15A0014	6 Jul 23	6 Jul 31	-
20	Vibration Meter	Vibration Level Acceleration Level	Instantel Inc.	Micromate UM14546	Calibration Laboratory Co.Ltd	Q24127999A1	4 Dec 24	3 Dec 25	-
21	Vibration Meter	Vibration Level Acceleration Level	Instantel Inc.	Micromate UM14466	Calibration Laboratory Co.Ltd	Q24128001A1	4 Dec 24	3 Dec 25	-
22	Vibration Meter	Vibration Level Acceleration Level	Instantel Inc.	Micromate UM14467	Calibration Laboratory Co.Ltd	Q24128000A1	4 Dec 24	3 Dec 25	-
23	Vibration Meter	Vibration Level Acceleration Level	Instantel Inc.	Micromate UM14472	Calibration Laboratory Co.Ltd	Q24127998A1	4 Dec 24	3 Dec 25	-
24	Sound Level Calibrator (Acoustic Calibrator)	Calibrate Sound Level Meter	01dB	CAL31 84065	Innovative Instrument Co.,Ltd.	24-ACT-087	25 Jun 24	24 Jun 25	-
25	Sound Level Meter	$L_{Aeq\ 24\ hrs}$, $L_{Aeq\ 1\ hr}$, L_{Amax} , L_{A90} , L_{Adn}	Larson Davis	LxT2 0006691	Innovative Instrument Co.,Ltd.	24-SLM-236	10 Jul 24	9 Jul 25	-
26	Sound Level Meter	$L_{Aeq\ 24\ hrs}$, $L_{Aeq\ 1\ hr}$, L_{Amax} , L_{A90} , L_{Adn}	Larson Davis	LxT2 0005372	Innovative Instrument Co.,Ltd.	24-SLM-229	9 Jul 24	8 Jul 25	-
27	Sound Level Meter	$L_{Aeq\ 24\ hrs}$, $L_{Aeq\ 1\ hr}$, L_{Amax} , L_{A90} , L_{Adn}	Larson Davis	LxT2 0006756	Innovative Instrument Co.,Ltd.	24-SLM-239	11 Jul 24	10 Jul 25	-
28	Sound Level Meter	$L_{Aeq\ 24\ hrs}$, $L_{Aeq\ 1\ hr}$, L_{Amax} , L_{A90} , L_{Adn}	Larson Davis	LxT2 0006757	Electrical And Electronics Institute Foundation For Industrial Development	CP20240321EA	22 Aug 24	21 Aug 25	-

CERTIFICATE OF CALIBRATION

Certificate No. : COF-039-67

Page 1 of 2 Pages

MEASUREMENT ITEM : Top Load Orifice
MANUFACTURER : TISCH
MODEL/TYPE : TE-5025A
SERIAL NUMBER : 3383
ID NUMBER : UAE.EFM.063/2560
CONDITION AS-RECEIVED : Used Item
CUSTOMER : United Analyst and Engineering Consultant Co., Ltd.
81 Soi Udomsuk 41, Sukhumvit Road, Bangkok, Phrakhanong,
Bangkok 10260

RECEIVED DATE : 16 Sep 2024
MEASUREMENT DATE : 27 Sep 2024
ISSUE DATE : 27 Sep 2024

ENVIRONMENTAL CONDITIONS:
Ambient condition in the laboratory are as follows:
Temperature : 23.0 ± 3.0 °C
Relative Humidity : 55.0 ± 15.0 %RH
Atmospheric Pressure : 1010 ± 10 hPa

CALIBRATION CONDITION:
Preconditioning : 24 hours at ambient conditions.
Measurement Condition : The average values during measurement are 23.9 °C and 49.0 %RH.

NOTED: The certificate is valid only to the item calibrated on date and place of calibration.

TABULATION OF RESULTS:
The table on next page give the measured values.

Calibrated by:
☐ Mr. Sorawit Thachalad
☒ Miss Jittraporn Lertsomphol



Approved sign



MEASUREMENT RESULTS:

The Orifice gas flow device was calibrated by direct comparison method with the Standard Rotary Displacement Meter (Roots Meter). The Humid air was used as a medium in the system. The standard conditions are 25 °C (298.15 K) and 760 mmHg for standard temperature and standard pressure respectively.

Table 1: The results of Q standard calibration data

Plate	Flow rate m ³ /min	Pressure [Pa] mmHg	Temperature [Ta] °C	Temperature [Tm] °C	Ap_meter mmHg	Ap_Orifice inH ₂ O	γ	Standard Flow [Qs] m ³ /min
1	0.703	758.131	23.92	22.49	56.556	1.738	1.319	0.654
2	1.000	758.205	23.70	22.81	63.034	3.473	1.865	0.922
3	1.121	758.284	23.64	22.69	42.633	4.642	2.157	1.064
4	1.167	758.274	23.64	22.65	31.359	5.197	2.282	1.125
5	1.409	758.325	24.00	23.14	30.402	7.654	2.768	1.358

Slope (m): 2.05577
Intercept (b): -0.02807
Correlation coefficient (r): 0.99985
Uncertainty (k=2): 0.015 m³/min

Table 2: The results of Q actual calibration data

Plate	Flow rate m ³ /min	Pressure [Pa] mmHg	Temperature [Ta] °C	Temperature [Tm] °C	Ap_meter mmHg	Ap_Orifice inH ₂ O	γ	Standard Flow [Qs] m ³ /min
1	0.703	758.131	23.92	22.49	56.556	1.738	0.825	0.653
2	1.000	758.205	23.70	22.81	63.034	3.473	1.166	0.920
3	1.121	758.284	23.64	22.69	42.633	4.642	1.348	1.061
4	1.167	758.274	23.64	22.65	31.359	5.197	1.426	1.123
5	1.409	758.325	24.00	23.14	30.402	7.654	1.732	1.357

Slope (m): 1.28763
Intercept (b): -0.01756
Correlation coefficient (r): 0.99985
Uncertainty (k=2): 0.015 m³/min

End of Certificate of Calibration



THIS CERTIFICATE REPORT MAY NOT BE REPRODUCED EXCEPT IN FULL UNLESS PERMISSION FOR REPRODUCTION IS GRANTED BY THE LABORATORY

เอกสารไม่ควบคุม

เอกสารไม่ควบคุม



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG, BANGKOK 10250
TEL. 0-2717-3000-24 FAX. 0-2719-9484

Certificate of Calibration

Certificate No. : 25P112
Page : 1 of 2

Equipment : U-Tube Manometer
Manufacturer: Dwyer
Model : 121-36-W/M
Serial No.: -
ID No.: UAE.EFM.181/2561
Condition As-Received: Used Item
Received Date: 10 February 2025
Calibration Date: 19 February 2025
Reference: 2502-0083WSC
Ambient Temperature: (23 ± 2) °C
Relative Humidity: (50 ± 15) %
Atmospheric Pressure: 1012 mbar

Submitted by: United Analyst and Engineering Consultant Co.,Ltd.

81 Soi Udomsuk 41, Sukhumvit Road, Bangkok,
Phrakhanong, Bangkok 10260

Procedure used: The calibration was conducted by direct comparison method against Pressure Measuring Instruments Standard according to in-house calibration procedure CP-P04, using * DKD-R 6-1 ; Calibration of Pressure Gauges, Edition 03/2014 * as a guidelines.

Condition of this result of calibration

1. Reference standards instruments :

Instrument	Model	Serial No.	Certificate No.	Due Date
1) Pressure Calibrator	PC106P	1189	MP-0113-24	10 Jul 2025

- This result of calibration was made on requested at the point specified by customer.
- Scale and conversion factor is 1 kPa = 4.0146293 inH₂O
- This instrument was used clean air as pressure media.
- This instrument was installed in vertical orientation and center of connector was used as the reference level.
- The certificate is valid only to the item calibrated on date and place of calibration.
- This Certification is traceable to the International System of Unit maintained at:-
National Institute of Metrology Thailand (NIMT)



Cert.No.: 25P112
Page: 2 of 2

Result of calibration:- Without adjustment
Function:- Pressure Measurement
Increasing Pressure

Range: 0 inH₂O to 36 inH₂O
Scale Interval: 0.1 inH₂O (The Fifth Estimate)

UUC Indication				
Applied Pressure (inH ₂ O)	High-port side (inH ₂ O)	Low-port side (inH ₂ O)	ΔP (inH ₂ O)	Error (inH ₂ O)
0.00	0.00	0.00	0.00	0.00
2.00	1.00	-0.98	1.98	-0.02
4.00	2.00	-1.98	3.98	-0.02
6.00	3.00	-3.02	6.02	0.02
8.00	4.00	-4.02	8.02	0.02
10.00	5.00	-5.04	10.04	0.04
12.00	6.00	-6.04	12.04	0.04
14.00	7.00	-7.06	14.06	0.06
16.00	8.00	-8.06	16.06	0.06
18.00	9.00	-9.06	18.06	0.06
20.00	10.00	-10.06	20.06	0.06
22.00	11.00	-11.08	22.08	0.08
24.00	12.00	-12.08	24.08	0.08
26.00	13.02	-13.10	26.12	0.12
28.00	14.02	-14.10	28.12	0.12
30.00	15.02	-15.10	30.12	0.12
32.00	16.02	-16.10	32.12	0.12
34.00	17.02	-17.08	34.10	0.10
36.00	17.86	-17.92	35.78	0.28

The uncertainty of measurement was ± 0.11 inH₂O

* UUC = Unit Under Calibration

* ΔP = High-port side - Low-port side

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k = 2, providing a level of confidence of approximately 95 %.

-o0o-

เอกสารไม่ควบคุม
B 0250406

เอกสารไม่ควบคุม
a 1037943



Certificate of Calibration

Certificate No. : 24P1856
Page : 1 of 2

Equipment : Aneroid Barometer

Manufacturer : Barigo

Model : -

Serial No. : -

ID No. : UAE.EMA2.110/2555

Condition As-Received: Used Item

Received Date: 24 May 2024

Calibration Date: 04 June 2024

Reference: 2405-0919WSC

Ambient Temperature: (23 ± 2) °C

Relative Humidity: (50 ± 15) %

Atmospheric Pressure: 1006 mbar

Submitted by: United Analyst and Engineering Consultant Co.,Ltd.

81 Soi Udomsuk 41, Sukhumvit Road,
Bangchak, Phrakhanong, Bangkok 10260

Procedure used: The calibration was conducted by direct comparison method against Pressure Measuring Instruments Standard according to in-house calibration procedure CP-P10, using * DKD-R 6-1 ; Calibration of Pressure Gauges, Edition 03/2014 " as a guidelines.

Condition of this result of calibration

1.Reference standards instruments :

Instrument	Model	Serial No.	Certificate No.	Due Date
1) Standard Barometer	DPI142	1422505046	MP-0094-24	03 May 2025

2.This instrument was installed in vertical orientation and center of the dial was used as the reference level.

3.This result of calibration was made on requested at the point specified by customer.

4.This result of calibration instrument was in absolute pressure.

5.This instrument was used clean air as pressure media.

6.The certificate is valid only to the item calibrated on date and place of calibration.

7.This Certification is traceable to the International System of Unit maintained through:-

-National Institute of Metrology Thailand (NIMT)

Attapol Panurach

เอกสารไม่ควบคุม
B 0316956



Cert.No.: 24P1856
Page: 2 of 2

Result of calibration:- Without adjustment

Function:- Absolute Pressure Measurement

Range : 720 mmHg to 800 mmHg

Scale interval : 1 mmHg (The Fifth Estimate)

Increasing Pressure

Applied Pressure (mmHg)	720.43	730.67	740.34	751.52	756.56	761.83	773.53	798.76
UUC* Indication (mmHg)	720.0	730.0	740.0	750.0	755.0	760.0	770.0	790.0
Error (mmHg)	-0.43	-0.67	-0.34	-1.52	-1.56	-1.83	-3.53	-8.76

Decreasing Pressure

Applied Pressure (mmHg)	798.76	773.60	761.89	756.65	751.59	740.72	730.68	720.59
UUC* Indication (mmHg)	790.0	770.0	760.0	755.0	750.0	740.0	730.0	720.0
Error (mmHg)	-8.76	-3.60	-1.89	-1.65	-1.59	-0.72	-0.68	-0.59

The uncertainty of measurement was ± 0.24 mmHg

* UUC = Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k = 2, providing a level of confidence of approximately 95 %.

-000-

เอกสารไม่ควบคุม
a 1165502



Certificate of Calibration

Certificate No. : 24H1487
Page : 1 of 2

Equipment : Digital Thermo-Hygrometer

Manufacturer : Digicon

Model : TH-02A

Serial No. : 435031148

ID No. : UAE.EFM.006/2567

Condition As-Received: New Item

Received Date: 10 July 2024

Calibration Date: 15 July 2024

to 17 July 2024

Reference: 2407-0393WSC

Ambient Temperature: (25 ± 3) °C

Relative Humidity: (50 ± 20) %

Submitted by: United Analyst and Engineering Consultant Co.,Ltd.

81 Soi Udomsuk 41, Sukhumvit Road, Bangchak,
Phrakhanong, Bangkok 10260

Procedure used: Calibration were conducted using in-house calibration procedure CP-H03 according to comparison with standard chilled mirror sensor for humidity measurement function and comparison with standard temperature probe for temperature measurement function into humidity / temperature chamber.

Condition of this result of calibration

1.Reference standards instruments :

Instrument	Model	Serial No.	Certificate No.	Due Date
1) Standard Chilled Mirror Hygrometer Sensor	Dew Prime II	31863	21819	25 Sep 2024
2) Handheld Thermometer With Sensor	1523	5717096	2311321	08 Nov 2024

2.The certificate is valid only to the item calibrated on date and place of calibration.

3.This Certification is traceable to the International System of Unit maintained through:-

-Thunder Scientific Corporation, NVLAB Accreditation No. Calibration 200582-0

-Technology Promotion Association (Thailand-Japan), NSC-ONSC Accredited No. Calibration 0008

Unnophol Harachai

เอกสารไม่ควบคุม



Cert. No.: 24H1487
Page.: 2 of 2

Result of Calibration:- Without Adjustment

Function: Humidity Measurement.

Reference Temperature (°C)	Standard Humidity (%R.H.)	UUC* Reading (%R.H.)	Error (%R.H.)	Uncertainty of Measurement (±%R.H.)
25.0	40.1	39	-1.1	1.4
25.0	50.1	48	-2.1	1.6
25.0	60.0	58	-2.0	1.6
25.0	70.2	68	-2.2	1.6

Result of Calibration:- Without Adjustment

Function: Temperature Measurement.

Standard Temperature (°C)	UUC* Reading (°C)	Error (°C)	Uncertainty of Measurement (±°C)
20.014	20.3	0.286	0.42
24.984	25.2	0.216	0.42
30.050	30.1	0.050	0.42
40.027	40.0	-0.027	0.42

UUC* : Unit Under Calibration

The reported uncertainty of measurement was base on standard uncertainty multiplied by coverage factor k = 2.00, providing confidence level approximately 95%.

-000-

เอกสารไม่ควบคุม

MULTI-POINT GAS TEST REPORT


Test Date : Sep 20,2024

Equipment : Gas Analyzer (NO₂) Model : 42i
Manufacturer : Thermo Scientific Serial Number : CM19050148

Standard Gas Concentration			Dilutor Detail	
Sulphur Dioxide (SO ₂)	42.89	PPM	Manufacturer :	Thermo Scientific
Nitric Oxide (NO)	46.77	PPM	Model :	146i
Methane (CH ₄)	-	PPM	Serial Number :	1180540071
Carbon Monoxide (CO)	965.9			
Cylinder No. :	EB0159156			
Expiration Date :	Nov 6,2026			

Multi-point gas test data

Reference Value (ppb)			Analyzer Display (ppb)	Difference Error	Percent Error	[% Error]
Level 1	Zero	0.0	0.0	0.00	0.00	0.00
Level 2	20.00%	100.0	100.7	0.70	0.70	0.70
Level 3	40.00%	200.0	200.6	0.60	0.30	0.30
Level 4	60.00%	300.0	300.9	0.90	0.30	0.30
Level 5	80.00%	400.0	400.0	0.00	0.00	0.00
Remark : Measuring Range			500.0 ppb	Average Difference (%)		0.26

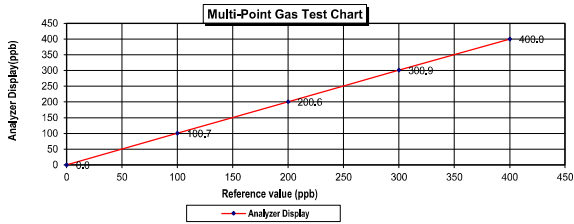

MULTI-POINT GAS TEST REPORT


Test Date : Sep 17,2024

Equipment : Gas Analyzer (NO₂) Model : 42i
Manufacturer : Thermo Scientific Serial Number : CM19050149

Standard Gas Concentration			Dilutor Detail	
Sulphur Dioxide (SO ₂)	42.89	PPM	Manufacturer :	Thermo Scientific
Nitric Oxide (NO)	46.77	PPM	Model :	146i
Methane (CH ₄)	-	PPM	Serial Number :	1180540071
Carbon Monoxide (CO)	965.9			
Cylinder No. :	EB0159156			
Expiration Date :	Nov 6,2026			

Multi-point gas test data

Reference Value (ppb)			Analyzer Display (ppb)	Difference Error	Percent Error	[% Error]
Level 1	Zero	0.0	0.0	0.00	0.00	0.00
Level 2	20.00%	100.0	100.8	0.80	0.79	0.79
Level 3	40.00%	200.0	200.6	0.60	0.30	0.30
Level 4	60.00%	300.0	300.7	0.70	0.23	0.23
Level 5	80.00%	400.0	400.0	0.00	0.00	0.00
Remark : Measuring Range			500.0 ppb	Average Difference (%)		
				0.27		

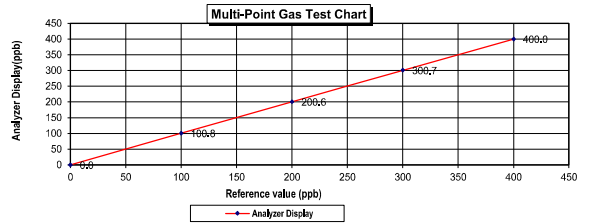

MULTI-POINT GAS TEST REPORT


Test Date : Oct 4,2024

Equipment : Gas Analyzer (NO₂) Model : 42i
Manufacturer : Thermo Scientific Serial Number : CM22387036

Standard Gas Concentration			Dilutor Detail	
Sulphur Dioxide (SO ₂)	42.89	PPM	Manufacturer :	Thermo Scientific
Nitric Oxide (NO)	46.77	PPM	Model :	146i
Methane (CH ₄)	-	PPM	Serial Number :	1180540071
Carbon Monoxide (CO)	965.9			
Cylinder No. :	EB0159156			
Expiration Date :	Nov 6,2026			

Multi-point gas test data

Reference Value (ppb)			Analyzer Display (ppb)	Difference Error	Percent Error	[% Error]
Level 1	Zero	0.0	0.0	0.00	0.00	0.00
Level 2	20.00%	100.0	100.7	0.70	0.70	0.70
Level 3	40.00%	200.0	201.3	1.30	0.65	0.65
Level 4	60.00%	300.0	300.9	0.90	0.30	0.30
Level 5	80.00%	400.0	400.0	0.00	0.00	0.00
Remark : Measuring Range		500.0 ppb	Average Difference (%)			0.33

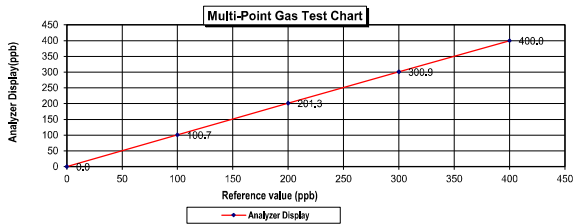

MULTI-POINT GAS TEST REPORT


Test Date : Oct 4,2024

Equipment : Gas Analyzer (NO₂) Model : 42i
Manufacturer : Thermo Scientific Serial Number : CM22387037

Standard Gas Concentration			Dilutor Detail	
Sulphur Dioxide (SO ₂)	42.89	PPM	Manufacturer :	Thermo Scientific
Nitric Oxide (NO)	46.77	PPM	Model :	146i
Methane (CH ₄)	-	PPM	Serial Number :	1180540071
Carbon Monoxide (CO)	965.9			
Cylinder No. :	EB0159156			
Expiration Date :	Nov 6,2026			

Multi-point gas test data

Reference Value (ppb)			Analyzer Display (ppb)	Difference Error	Percent Error	[% Error]
Level 1	Zero	0.0	0.0	0.00	0.00	0.00
Level 2	20.00%	100.0	100.8	0.80	0.79	0.79
Level 3	40.00%	200.0	200.7	0.70	0.35	0.35
Level 4	60.00%	300.0	301.5	1.50	0.50	0.50
Level 5	80.00%	400.0	400.0	0.00	0.00	0.00
Remark : Measuring Range 500.0 ppb			Average Difference (%) 0.33			

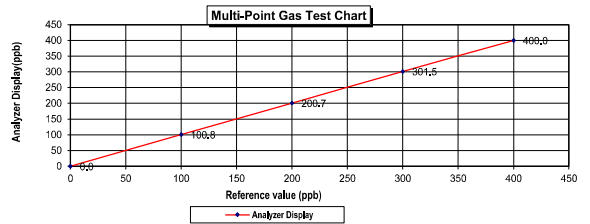

CERTIFICATE OF ANALYSIS

Grade of Product: EPA PROTOCOL STANDARD

Customer: AIR LIQUIDE (THAILAND)
LTD--
Part Number: E05NI91E15A0014 Reference Number: 160-40272205-1
Cylinder Number: EB0162121 Cylinder Volume: 144.0 CF
Laboratory: 124 - Plumsteadville - PA Cylinder Pressure: 2016 PSIG
PGVP Number: A12023 Valve Outlet: 660
Gas Code: CO, CO2, NO, NOX, SO2, BALN Certification Date: Jul 06, 2023

Expiration Date: Jul 06, 2031

Certification performed in accordance with "EPA Traceability Protocol" for Assay and Certification of Gaseous Calibration Standards (May 2012) document EPA 800/R-12/531, using the assay procedures listed. Analytical Methodology does not require correction for analytical interference. This cylinder has a total analytical uncertainty as stated below with a confidence level of 95%. There are no significant impurities which affect the use of this calibration mixture. All concentrations are on a mole/mole basis unless otherwise noted. The results relate only to the items tested. The report shall not be reproduced except in full without approval of the laboratory. Do Not Use This Cylinder below 100 psig, i.e. 0.7 megapascals.

ANALYTICAL RESULTS					
Component	Requested Concentration	Actual Concentration	Protocol Method	Total Relative Uncertainty	Assay Dates
NOX	100.0 PPM	100.4 PPM	G1	+/- 0.9% NIST Traceable	06/27/2023, 07/06/2023
NITRIC OXIDE	100.0 PPM	100.2 PPM	G1	+/- 0.9% NIST Traceable	06/27/2023, 07/06/2023
SULFUR DIOXIDE	100.0 PPM	100.0 PPM	G1	+/- 1.4% NIST Traceable	06/27/2023, 07/06/2023
CARBON MONOXIDE	200.0 PPM	199.2 PPM	G1	+/- 0.3% NIST Traceable	06/26/2023
CARBON DIOXIDE	8.000 %	7.982 %	G1	+/- 1.2% NIST Traceable	06/27/2023
NITROGEN	Balance				

CALIBRATION STANDARDS					
Type	Lot ID	Cylinder No	Concentration	Uncertainty	Expiration Date
GMIS	104202308	CC754364	98.36 PPM NITRIC OXIDE/NITROGEN	+/- 0.4%	Jan 04, 2031
PRM	C2219101	APE1514048	100.19 PPM NITRIC OXIDE/NITROGEN	+/- 0.3%	Feb 28, 2025
GMIS	2023042525	CC754381	98.52 PPM NITRIC OXIDE/NITROGEN	+/- 0.4%	Apr 25, 2031
PRM	12409	D913660	15.01 PPM NITROGEN DIOXIDE/AIR	+/- 1.5%	Feb 17, 2023
GMIS	153400202002	EB0130037	9.693 PPM NITROGEN DIOXIDE/NITROGEN	+/- 1.6%	Sep 29, 2025
NTRM	160102-22	KAL003820	97.69 PPM SULFUR DIOXIDE/NITROGEN	+/- 0.8%	Nov 01, 2027
CO	230601	CC745902	249.47 PPM CARBON MONOXIDE/NITROGEN	+/- 0.3%	Dec 09, 2028
NTRM	130606-02	CC411730	13.359 % CARBON DIOXIDE/NITROGEN	+/- 0.6%	May 14, 2025

The SRM, NTRM, PRM, or RGM noted above is only in reference to the GMIS used in the assay and not part of the analysis.

ANALYTICAL EQUIPMENT			
Instrument/Make/Model	Analytical Principle	Last Multipoint Calibration	
Nicolet iS50 FTIR AUP2010245 CO2	FTIR	Jun 15, 2023	
SIEMENS ULTRAMAT6E N1-C8-180	NDIR	Jun 14, 2023	
Nicolet iS50 FTIR AUP2010245 NO	FTIR	Jun 29, 2023	
Nicolet iS50 FTIR AUP2010245 NOX	FTIR	Jun 15, 2023	
Nicolet iS50 FTIR AUP2010245 SO2	FTIR	Jun 08, 2023	



Page 1 of 1

เอกสารไม่ควบคุม

MULTI-POINT GAS TEST REPORT

Test Date : Sep 6, 2024



Equipment : Gas Analyzer (SO₂) Model : 43i
Manufacturer : Thermo SCIENTIFIC Serial Number : CM22387061

Standard Gas Concentration			Dilutor Detail	
Sulphur Dioxide (SO ₂)	42.89	PPM	Manufacturer :	Thermo SCIENTIFIC
Nitric Oxide (NO)	46.77	PPM	Model :	146i
Methane (CH ₄)	-	PPM	Serial Number :	1180540071
Carbon Monoxide (CO)	965.9			
Cylinder No. :	EB01159156			
Expiration Date :	Nov 06, 2026			

Multi-point gas test data

	Reference Value (ppb)		Analyzer Display (ppb)	Difference Error	Percent Error	[% Error]
Level 1	Zero	0.0	0.0	0.00	0.00	0.00
Level 2	20.00%	100.0	100.7	0.70	0.70	0.70
Level 3	40.00%	200.0	200.7	0.70	0.35	0.35
Level 4	60.00%	300.0	301.1	1.10	0.37	0.37
Level 5	80.00%	400.0	400.0	0.00	0.00	0.00

Remark : Measuring Range : 500.0 ppb
:Acceptable Limit \pm 5%

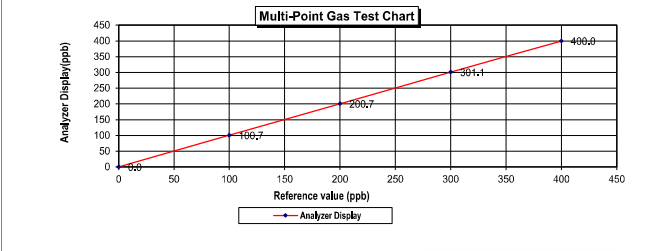

Page 1 of 1

เอกสารไม่ควบคุม

MULTI-POINT GAS TEST REPORT

Test Date : June 19, 2024


Equipment : Gas Analyzer (SO₂) Model : 43i
Manufacturer : Thermo SCIENTIFIC Serial Number : CM22387063

Standard Gas Concentration			Dilutor Detail	
Sulphur Dioxide (SO ₂)	42.89	PPM	Manufacturer :	Thermo SCIENTIFIC
Nitric Oxide (NO)	46.77	PPM	Model :	146i
Methane (CH ₄)	-	PPM	Serial Number :	1180540071
Carbon Monoxide (CO)	965.9			
Cylinder No. :	EB0159156			
Expiration Date :	Nov 06, 2026			

Multi-point gas test data

	Reference Value (ppb)		Analyzer Display (ppb)	Difference Error	Percent Error	[% Error]
Level 1	Zero	0.0	0.0	0.00	0.00	0.00
Level 2	20.00%	100.0	100.8	0.80	0.79	0.79
Level 3	40.00%	200.0	200.7	0.70	0.35	0.35
Level 4	60.00%	300.0	301.1	1.10	0.37	0.37
Level 5	80.00%	400.0	400.0	0.00	0.00	0.00

Remark : Measuring Range : 500.0 ppb
:Acceptable Limit \pm 5%

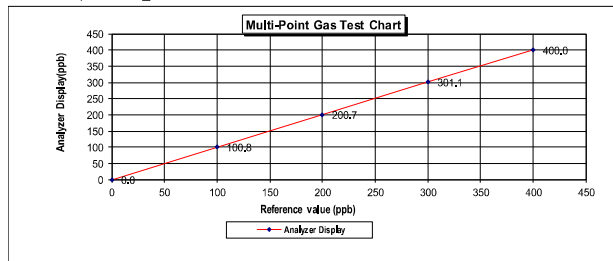

Page 1 of 1

เอกสารไม่ควบคุม

MULTI-POINT GAS TEST REPORT

Test Date : Sep 6, 2024


Equipment : Gas Analyzer (SO₂) Model : 43i
Manufacturer : Thermo SCIENTIFIC Serial Number : CM22387065

Standard Gas Concentration			Dilutor Detail	
Sulphur Dioxide (SO ₂)	42.89	PPM	Manufacturer :	Thermo SCIENTIFIC
Nitric Oxide (NO)	46.77	PPM	Model :	146i
Methane (CH ₄)	-	PPM	Serial Number :	1180540071
Carbon Monoxide (CO)	965.9			
Cylinder No. :	EB01159156			
Expiration Date :	Nov 06, 2026			

Multi-point gas test data

	Reference Value (ppb)		Analyzer Display (ppb)	Difference Error	Percent Error	[% Error]
Level 1	Zero	0.0	0.0	0.00	0.00	0.00
Level 2	20.00%	100.0	100.6	0.60	0.60	0.60
Level 3	40.00%	200.0	200.6	0.60	0.30	0.30
Level 4	60.00%	300.0	300.9	0.90	0.30	0.30
Level 5	80.00%	400.0	400.0	0.00	0.00	0.00

Remark : Measuring Range : 500.0 ppb
:Acceptable Limit \pm 5%

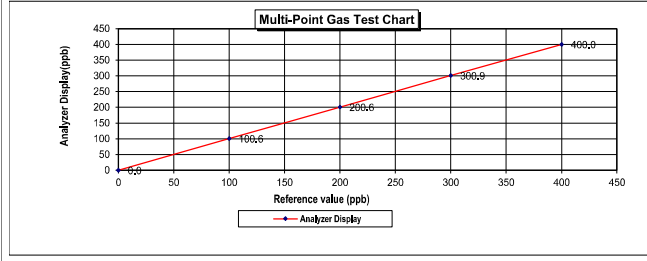

Page 1 of 1

เอกสารไม่ควบคุม

MULTI-POINT GAS TEST REPORT


Test Date : Sep 6, 2024

Equipment : Gas Analyzer (SO₂) Model : 43i
Manufacturer : Thermo SCIENTIFIC Serial Number : CM22387066

Standard Gas Concentration			Dilutor Detail	
Sulphur Dioxide (SO ₂)	42.89	PPM	Manufacturer :	Thermo SCIENTIFIC
Nitric Oxide (NO)	46.77	PPM	Model :	146i
Methane (CH ₄)	-	PPM	Serial Number :	1180540071
Carbon Monoxide (CO)	965.9			
Cylinder No. :	EB01159156			
Expiration Date :	Nov 06, 2026			

Multi-point gas test data

Reference Value (ppb)			Analyzer Display (ppb)	Difference Error	Percent Error	[% Error]
Level 1	Zero	0,0	0,0	0,00	0,00	0,00
Level 2	20.00%	100,0	100,9	0,90	0,89	0,89
Level 3	40.00%	200,0	200,7	0,70	0,35	0,35
Level 4	60.00%	300,0	300,7	0,70	0,23	0,23
Level 5	80.00%	400,0	400,0	0,00	0,00	0,00
Remark : Measuring Range			500.0 ppb	Average Difference (%)		0.29

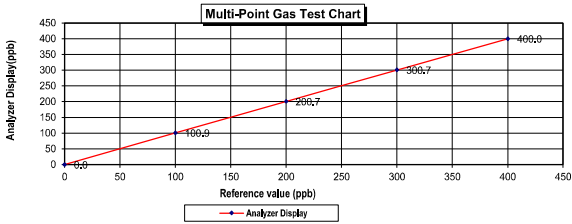

เอกสารไม่ควบคุม

CERTIFICATE OF ANALYSIS

Grade of Product: EPA PROTOCOL STANDARD

Customer: AIR LIQUIDE (THAILAND)

Part Number: E05NI91E15A0014 Reference Number: 160-402772205-1
Cylinder Number: EB0162121 Cylinder Volume: 144.0 CF
Laboratory: 124 - Plumsteadville - PA Cylinder Pressure: 2016 PSIG
PGVP Number: A12023 Valve Outlet: 660
Gas Code: CO,CO₂,NO,NO₂,SO₂,BALN Certification Date: Jul 06, 2023

Expiration Date: Jul 06, 2031

Certification performed in accordance with "EPA Traceability Protocol for Assay and Certification of Gaseous Calibration Standards (May 2012)" document EPA 800/R-12/531, using the assay procedures listed. Analytical Methodology does not require correction for analytical interference. This cylinder has a total analytical uncertainty as stated below with a confidence level of 95%. There are no significant impurities which affect the use of this calibration mixture. All concentrations are on a mole/mole basis unless otherwise noted. The results relate only to the items tested. The report shall not be reproduced except in full without approval of the laboratory. Do Not Use This Cylinder below 100 psig, i.e. 0.7 megapascals.

ANALYTICAL RESULTS					
Component	Requested Concentration	Actual Concentration	Protocol Method	Total Relative Uncertainty	Assay Dates
NOX	100.0 PPM	100.4 PPM	G1	+/- 0.9% NIST Traceable	06/27/2023, 07/06/2023
NITRIC OXIDE	100.0 PPM	100.2 PPM	G1	+/- 0.9% NIST Traceable	06/27/2023, 07/06/2023
SULFUR DIOXIDE	100.0 PPM	100.0 PPM	G1	+/- 1.4% NIST Traceable	06/27/2023, 07/06/2023
CARBON MONOXIDE	200.0 PPM	199.2 PPM	G1	+/- 0.3% NIST Traceable	06/26/2023
CARBON DIOXIDE	8.000 %	7.982 %	G1	+/- 1.2% NIST Traceable	06/27/2023
NITROGEN	Balance				

CALIBRATION STANDARDS					
Type	Lot ID	Cylinder No	Concentration	Uncertainty	Expiration Date
GMIS	104202308	CC754364	98.36 PPM NITRIC OXIDE/NITROGEN	+/- 0.4%	Jan 04, 2031
PRM	22219101	AP1514048	100.19 PPM NITRIC OXIDE/NITROGEN	+/- 0.3%	Feb 28, 2025
GMIS	2023042525	CC754381	98.52 PPM NITRIC OXIDE/NITROGEN	+/-0.4%	Apr 25, 2031
PRM	12409	D913660	15.01 PPM NITROGEN DIOXIDE/AIR	+/- 1.5%	Feb 17, 2023
GMIS	15340020002	EB0130037	9.693 PPM NITROGEN DIOXIDE/NITROGEN	+/- 1.6%	Sep 29, 2025
NTRM	160102-22	KAL003820	97.69 PPM SULFUR DIOXIDE/NITROGEN	+/- 0.8%	Nov 01, 2027
CO	230601	CC745902	249.47 PPM CARBON MONOXIDE/NITROGEN	+/- 0.3%	Dec 09, 2028
NTRM	133608-02	CC4117130	13.359 % CARBON DIOXIDE/NITROGEN	+/- 0.6%	May 14, 2025
The SRM, NTRM, PRM, or RGM noted above is only in reference to the GMIS used in the assay and not part of the analysis.					

ANALYTICAL EQUIPMENT		
Instrument/Make/Model	Analytical Principle	Last Multipoint Calibration
Nicolet iS50 FTIR AUP2010245 CO ₂	FTIR	Jun 15, 2023
SIEMENS ULTRAMAT6E N1-C8-180	NDIR	Jun 14, 2023
Nicolet iS50 FTIR AUP2010245 NO	FTIR	Jun 29, 2023
Nicolet iS50 FTIR AUP2010245 NO ₂	FTIR	Jun 15, 2023
Nicolet iS50 FTIR AUP2010245 SO ₂	FTIR	Jun 08, 2023

เอกสารไม่ควบคุม

MULTI-POINT GAS TEST REPORT


Test Date : Sep 9, 2024

Equipment : Gas Analyzer (CO) Model : 48i
Manufacturer : Thermo Scientific Serial Number : 1200906880

Standard Gas Concentration			Dilutor Detail	
Sulphur Dioxide (SO ₂)	42.89	PPM	Manufacturer :	Thermo Scientific
Nitric Oxide (NO)	46.77	PPM	Model :	146i
Methane (CH ₄)	-	PPM	Serial Number :	1180540071
Carbon Monoxide (CO)	965.9	PPM		
Cylinder No. :	EB01159156			
Expiration Date :	Nov 06, 2026			

Multi-point gas test data

Reference Value (ppm)			Analyzer Display (ppm)	Difference Error	Percent Error	[% Error]
Level 1	Zero	0,0	0,0	0,0	0,0	0,0
Level 2	20.00%	10,0	10,7	0,7	6,5	6,5
Level 3	40.00%	20,0	20,9	0,9	4,3	4,3
Level 4	60.00%	30,0	30,7	0,7	2,3	2,3
Level 5	80.00%	40,0	40,0	0,0	0,0	0,0
Remark : Measuring Range			50.0 ppm	Average Difference (%)		2.63

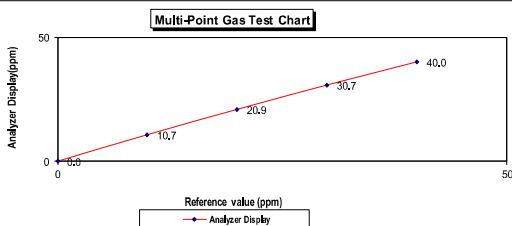

เอกสารไม่ควบคุม

MULTI-POINT GAS TEST REPORT


Test Date : Sep 9, 2024

Equipment : Gas Analyzer (CO) Model : 48i
Manufacturer : Thermo Scientific Serial Number : 1201497730

Standard Gas Concentration			Dilutor Detail	
Sulphur Dioxide (SO ₂)	42.89	PPM	Manufacturer :	Thermo Scientific
Nitric Oxide (NO)	46.77	PPM	Model :	146i
Methane (CH ₄)	-	PPM	Serial Number :	1180540071
Carbon Monoxide (CO)	965.9	PPM		
Cylinder No. :	EB01159156			
Expiration Date :	Nov 06, 2026			

Multi-point gas test data

Reference Value (ppm)			Analyzer Display (ppm)	Difference Error	Percent Error	[% Error]
Level 1	Zero	0,0	0,0	0,0	0,0	0,0
Level 2	20.00%	10,0	10,6	0,6	5,7	5,7
Level 3	40.00%	20,0	20,9	0,9	4,3	4,3
Level 4	60.00%	30,0	30,8	0,8	2,6	2,6
Level 5	80.00%	40,0	40,0	0,0	0,0	0,0
Remark : Measuring Range		50.0 ppm	Average Difference (%)			2,51

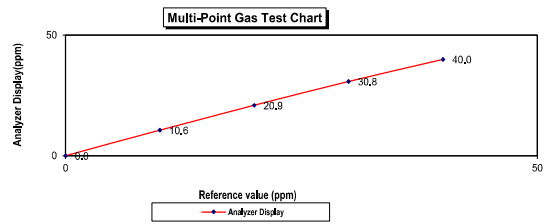

เอกสารไม่ควบคุม

MULTI-POINT GAS TEST REPORT

Test Date : Sep 9, 2024

Equipment : Gas Analyzer (CO) Model : 48i
Manufacturer : Thermo Scientific Serial Number : 1201497732

Standard Gas Concentration


Sulphur Dioxide (SO₂) 42.89 PPM
Nitric Oxide (NO) 46.77 PPM
Methane (CH₄) - PPM
Carbon Monoxide (CO) 965.9 PPM
Cylinder No. : EB01159156
Expiration Date : Nov 06, 2026

Dilutor Detail

Manufacturer : Thermo Scientific
Model : 146i
Serial Number : 1180540071

Multi-point gas test data

	Reference Value (ppm)	Analyzer Display (ppm)	Difference Error	Percent Error	[% Error]
Level 1	Zero	0.0	0.0	0.0	0.0
Level 2	20.00%	10.0	10.6	0.5	5.7
Level 3	40.00%	20.0	20.5	0.5	2.4
Level 4	60.00%	30.0	30.9	0.9	2.9
Level 5	80.00%	40.0	40.0	0.0	0.0
Remark : Measuring Range	50.0 ppm		Average Difference (%)		2.20
:Acceptable Limit \pm 5%					

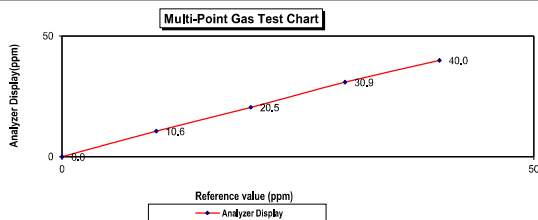

Page 1 of 1

เอกสารไม่ควบคุม

MULTI-POINT GAS TEST REPORT

Test Date : June 14, 2024

Equipment : Gas Analyzer (CO) Model : 48i
Manufacturer : Thermo Scientific Serial Number : 1201497733

Standard Gas Concentration


Sulphur Dioxide (SO₂) 42.89 PPM
Nitric Oxide (NO) 46.77 PPM
Methane (CH₄) - PPM
Carbon Monoxide (CO) 965.9 PPM
Cylinder No. : EB01159156
Expiration Date : Nov 06, 2026

Dilutor Detail

Manufacturer : Thermo Scientific
Model : 146i
Serial Number : 1180540071

Multi-point gas test data

	Reference Value (ppm)	Analyzer Display (ppm)	Difference Error	Percent Error	[% Error]
Level 1	Zero	0.0	0.0	0.0	0.0
Level 2	20.00%	10.0	10.5	0.5	4.8
Level 3	40.00%	20.0	20.5	0.5	2.4
Level 4	60.00%	30.0	30.9	0.9	2.9
Level 5	80.00%	40.0	40.0	0.0	0.0
Remark : Measuring Range	50.0 ppm		Average Difference (%)		2.02
:Acceptable Limit \pm 5%					

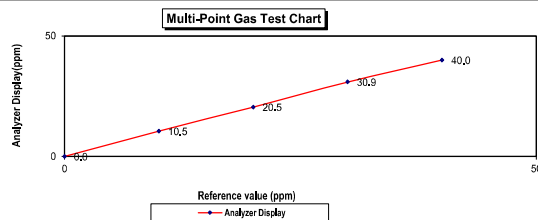

Page 1 of 1

เอกสารไม่ควบคุม



Airgas Specialty Gases
Airgas USA LLC
6141 Easton Road
Plumsteadville, PA 18949
Airgas.com

CERTIFICATE OF ANALYSIS

Grade of Product: EPA PROTOCOL STANDARD

Customer: AIR LIQUIDE (THAILAND)
LTD--
Part Number: E05NI91E15A0014
Cylinder Number: EB0162121
Laboratory: 124 - Plumsteadville - PA
PGVP Number: A12023
Gas Code: CO, CO₂, NO, NO₂, SO₂, BALN
Reference Number: 160-402772205-1
Cylinder Volume: 144.0 CF
Cylinder Pressure: 2016 PSIG
Valve Outlet: 660
Certification Date: Jul 06, 2031

Expiration Date: Jul 06, 2031

Certification performed in accordance with "EPA Traceability Protocol for Assay and Certification of Gaseous Calibration Standards" (May 2012) document EPA 800/R-12/531, using the assay procedures listed. Analytical Methodology does not require correction for analytical interference. This cylinder has a total analytical uncertainty as stated below with a confidence level of 95%. There are no significant impurities which affect the use of this calibration mixture. All concentrations are on a mole/mole basis unless otherwise noted. The results relate only to the items listed. The report shall not be reproduced except in full without approval of the laboratory. Do Not Use This Cylinder below 100 psig, i.e. 0.7 megapascals.

Component	Requested Concentration	Actual Concentration	Protocol Method	Total Relative Uncertainty	Assay Dates
NOX	100.0 PPM	100.4 PPM	G1	+/- 0.9% NIST Traceable	06/27/2023, 07/06/2023
NITRIC OXIDE	100.0 PPM	100.2 PPM	G1	+/- 0.9% NIST Traceable	06/27/2023, 07/06/2023
SULFUR DIOXIDE	100.0 PPM	100.0 PPM	G1	+/- 1.4% NIST Traceable	06/27/2023, 07/06/2023
CARBON MONOXIDE	200.0 PPM	199.2 PPM	G1	+/- 0.3% NIST Traceable	06/26/2023
CARBON DIOXIDE	8.000 %	7.982 %	G1	+/- 1.2% NIST Traceable	06/27/2023
NITROGEN	Balance				

CALIBRATION STANDARDS

Type	Lot ID	Cylinder No	Concentration	Uncertainty	Expiration Date
GMIS	104202308	CC754364	98.36 PPM NITRIC OXIDE/NITROGEN	+/- 0.4%	Jan 04, 2031
PRM	C2219101	APE1514048	100.19 PPM NITRIC OXIDE/NITROGEN	+/- 0.3%	Feb 28, 2025
GMIS	2023042525	CC754381	98.52 PPM NITRIC OXIDE/NITROGEN	+/-0.4%	Apr 25, 2031
PRM	12409	D913660	15.01 PPM NITROGEN DIOXIDE/AIR	+/- 1.5%	Feb 17, 2023
GMIS	153400202002	EB0130037	9.693 PPM NITROGEN DIOXIDE/NITROGEN	+/- 1.6%	Sep 29, 2025
NTRM	160102-22	KAL003820	97.69 PPM SULFUR DIOXIDE/NITROGEN	+/- 0.8%	Nov 01, 2027
CO	230601	CC745902	249.47 PPM CARBON MONOXIDE/NITROGEN	+/- 0.3%	Dec 09, 2028
NTRM	130606-02	CC411730	13.359 % CARBON DIOXIDE/NITROGEN	+/- 0.6%	May 14, 2025

The SRM, NTRM, PRM, or RGM noted above is only in reference to the GMIS used in the assay and not part of the analysis.

ANALYTICAL EQUIPMENT

Instrument/Make/Model	Analytical Principle	Last Multipoint Calibration
Nicolet iS50 FTIR AUP2010245 CO2	FTIR	Jun 15, 2023
SIEMENS ULTRAMATE6E N1-C8-180	NDIR	Jun 14, 2023
Nicolet iS50 FTIR AUP2010245 NO	FTIR	Jun 29, 2023
Nicolet iS50 FTIR AUP2010245 NO2	FTIR	Jun 15, 2023
Nicolet iS50 FTIR AUP2010245 SO2	FTIR	Jun 08, 2023



CALIBRATION LABORATORY CO., LTD.

2/10-11/14/55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



Supplement to Calibration Certificate No. Q24127999

CERTIFICATE OF CALIBRATION

FOR

NOMENCLATURE : VIBRATION METER
MANUFACTURER : INSTANTEL
MODEL / TYPE : 721A2601/721A3301
SERIAL NO. : UM14546/UM14546 [UAE.EFM.030/2562]
CLID. NO. : 252000247
JOB CONTROL NO. : 241203127999
CALIBRATION SERVICE : ☒ IN-LABORATORY ☐ ON-SITE

CUSTOMER : UNITED ANALYST AND ENGINEERING CONSULTANT CO., LTD.
81 SOI UDOMSUK 41, SUKHUMVIT ROAD,
BANGCHAK, PHRAKHANONG, BANGKOK 10260

DATE OF RECEIVED : 03 December 2024

DATE OF ISSUED : 29 January 2025

The report of calibration shall not be reproduced except in full without approval of the Calibration Laboratory Co., Ltd.

Calibrated By :

Approved By :

This Calibration Certificate documents

International System of Units (SI)

Certificate No. Q24127999A1

F3-012-05/12-23

page 1 of 4

เอกสารไม่ควบคุม

เอกสารไม่ควบคุม





CALIBRATION LABORATORY Co.,LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



Supplement to Calibration Certificate No. Q24127999

REPORT OF CALIBRATION

FOR

NOMENCLATURE : VIBRATION METER
MANUFACTURER : INSTANTEL
MODEL / TYPE : 721A2601/721A3301
SERIAL NO. : UM14546/UM14546 [UAE.EFM.030/2562]
DATE OF CALIBRATION : 04 December 2024

ENVIRONMENT CONDITIONS :

Temperature : (23 ± 2) °C Relative Humidity : (55 ± 15) %RH

PROCEDURE USED :

This instrument was calibrated under procedure No. CLC-CPEE-08 based on ISO 16063-21 as calibration guideline.

The calibration was performed by using Digital Multimeter, Programmable Timer/Counter, Vibration Calibrator which maintained by the Calibration Laboratory Co., Ltd.

REFERENCE STANDARD USED :

1. Vibration Calibrator, The Modal Shop Model 9110D S/N. 11424.
2. Programmable Timer/Counter, Philips Model PM6680B S/N. SM607101.
3. Digital Multimeter, Keysight Technologies Model 3458A S/N. MY59352733.

TRACEABILITY :

1. The measurements are traceable to International System of Units (SI), through National Institute of Metrology (Thailand) Certificate No. AV-0030-24, Due Date 19 July 2025.
2. The measurements are traceable to International System of Units (SI), through Aeronautical Radio of Thailand Ltd. Certificate No. 07-0050/24, Due Date 13 May 2025.
3. The measurements are traceable to International System of Units (SI), through National Institute of Metrology (Thailand) Certificate No. EE-0060-24, Due Date 26 June 2025.

UNCERTAINTY :

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor $k = 2.00$ which for a normal distribution corresponds to a coverage probability of approximately 95 %.

It has been evaluated according to the "Evaluation of the Uncertainty of Measurement in Calibration (EA-4/02 M:2022)"

Certificate No. Q24127999A1

F3-012-05/12-23

page 2 of 4

เอกสารไม่ควบคุม



@clccalibration



CALIBRATION LABORATORY Co.,LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



CONDITION OF CALIBRATION ITEM : RECEIVED IN GOOD OPERATIONAL CONDITION

MEASUREMENT RESULTS : (X) without adjustment () adjustment

CALIBRATION DATA

1. ACCELERATION RESULT

Test point		Mode	STD Reading	DUC Reading	Correction	Uncertainty
(g)	(frequency)		(g)	(g)	(g)	± (% of rdg.)
0.3	50 Hz	peak	0.300	0.305	-0.005	1.9
0.4	50 Hz		0.400	0.407	-0.007	1.6
0.5	50 Hz		0.500	0.508	-0.008	1.6
0.6	50 Hz		0.600	0.609	-0.009	2.5
0.7	50 Hz		0.700	0.710	-0.010	2.5
0.3	100 Hz	peak	0.300	0.304	-0.004	1.9
0.4	100 Hz		0.400	0.406	-0.006	1.6
0.5	100 Hz		0.500	0.508	-0.008	1.6
0.6	100 Hz		0.600	0.608	-0.008	2.5
0.7	100 Hz		0.700	0.709	-0.009	2.5

2. VELOCITY RESULT

Test point		Mode	STD Reading	DUC Reading	Correction	Uncertainty
(mm/s)	(frequency)		(mm/s)	(mm/s)	(mm/s)	± (% of rdg.)
3	50 Hz	peak	3.000	3.047	-0.047	1.8
4	50 Hz		4.000	4.054	-0.054	1.8
5	50 Hz		5.000	5.066	-0.066	1.8
6	50 Hz		6.000	6.079	-0.079	1.8
7	50 Hz		7.000	7.097	-0.097	1.8
*3	100 Hz	peak	3.000	3.045	-0.045	1.6
*4	100 Hz		4.000	4.066	-0.066	1.6
*5	100 Hz		5.000	5.075	-0.075	1.6
*6	100 Hz		6.000	6.088	-0.088	1.5
*7	100 Hz		7.000	7.101	-0.101	1.5

Certificate No. Q24127999

F3-011-05/12-23

page 3 of 4

เอกสารไม่ควบคุม



@clccalibration



CALIBRATION LABORATORY Co.,LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



CALIBRATION DATA

3. DISPLACEMENT RESULT

Test point		Mode	STD Reading	DUC Reading	Correction	Uncertainty
(mm)	(frequency)		(mm)	(mm)	(mm)	± (% of rdg.)
0.03	50 Hz	peak	0.030	0.030	0.000	2.5
0.04	50 Hz		0.040	0.040	0.000	2.1
0.05	50 Hz		0.050	0.050	0.000	1.9
0.06	50 Hz		0.060	0.061	-0.001	1.8
0.07	50 Hz		0.070	0.071	-0.001	1.8
0.03	100 Hz	peak	0.030	0.030	0.000	2.5
0.04	100 Hz		0.040	0.040	0.000	2.1
0.05	100 Hz		0.050	0.050	0.000	1.9
0.06	100 Hz		0.060	0.060	0.000	1.8
0.07	100 Hz		0.070	0.071	-0.001	1.8

Note. The Scope of Accredited ANAB Certificate No. ACDM-2814 Version 012 Page 1,2 of 67

* means Calibrations marked " Not ANAB Accredited " in this Certificate have been included for completeness.

This report is valid for the above stated instrument/s only.

End of Certificate

Certificate No. Q24127999

F3-011-05/12-23

page 4 of 4

เอกสารไม่ควบคุม



@clccalibration



CALIBRATION LABORATORY Co.,LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



Supplement to Calibration Certificate No. Q24128001

CERTIFICATE OF CALIBRATION

FOR

NOMENCLATURE : VIBRATION METER
MANUFACTURER : INSTANTEL
MODEL / TYPE : 721A2601/721A3301
SERIAL NO. : UM14466/UM14466 [UAE.EFM.095/2562]
CLID. NO. : 252000053
JOB CONTROL NO. : 241203128001
CALIBRATION SERVICE : ☒ IN-LABORATORY ☐ ON-SITE

CUSTOMER : UNITED ANALYST AND ENGINEERING CONSULTANT CO., LTD.

81 SOI UDOMSUH 41, SUKHUMVIT ROAD,
BANGCHAK, PHRAKHANONG, BANGKOK 10260

DATE OF RECEIVED : 03 December 2024

DATE OF ISSUED : 29 January 2025

The report of calibration shall not be reproduced except in full without approval of the Calibration Laboratory Co., Ltd.

Calibrated By :

Approved By :

This Calibration Certificate documents the

Certificate No. Q24128001A1

F3-012-05/12-23

page 1 of 4

เอกสารไม่ควบคุม



@clccalibration



Supplement to Calibration Certificate No. Q24128001

REPORT OF CALIBRATION

FOR

NOMENCLATURE : VIBRATION METER
MANUFACTURER : INSTANTEL
MODEL / TYPE : 721A2601/721A3301
SERIAL NO. : UM14466/UM14466 [UAE.EFM.095/2562]
DATE OF CALIBRATION : 04 December 2024

ENVIRONMENT CONDITIONS :

Temperature : (23 ± 2) °C Relative Humidity : (55 ± 15) %RH

PROCEDURE USED :

This instrument was calibrated under procedure No. CLC-CPEE-08 based on ISO 16063-21 as calibration guideline.
The calibration was performed by using Digital Multimeter, Programmable Timer/Counter, Vibration Calibrator which maintained by the Calibration Laboratory Co., Ltd.

REFERENCE STANDARD USED :

- Vibration Calibrator, The Modal Shop Model 9110D S/N. 11424.
- Programmable Timer/Counter, Philips Model PM6680B S/N. SM607101.
- Digital Multimeter, Keysight Technologies Model 3458A S/N. MY59352733.

TRACEABILITY :

- The measurements are traceable to International System of Units (SI), through National Institute of Metrology (Thailand) Certificate No. AV-0030-24, Due Date 19 July 2025.
- The measurements are traceable to International System of Units (SI), through Aeronautical Radio of Thailand Ltd. Certificate No. 07-0050/24, Due Date 13 May 2025.
- The measurements are traceable to International System of Units (SI), through National Institute of Metrology (Thailand) Certificate No. EE-0060-24, Due Date 26 June 2025.

UNCERTAINTY :

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor $k = 2.00$ which for a normal distribution corresponds to a coverage probability of approximately 95 %.

It has been evaluated according to the "Evaluation of the Uncertainty of Measurement in Calibration (EA-4/02 M:2022)"

Certificate No. Q24128001A1

F3-012-05/12-23

page 2 of 4

เอกสารไม่ควบคุม



@clccalibration

CONDITION OF CALIBRATION ITEM : RECEIVED IN GOOD OPERATIONAL CONDITION

MEASUREMENT RESULTS : (X) without adjustment () adjustment

CALIBRATION DATA

1. ACCELERATION RESULT

Test point		Mode	STD Reading	DUC Reading	Correction	Uncertainty
(g)	(frequency)		(g)	(g)	(g)	± (% of rdg.)
0.3	50 Hz	peak	0.300	0.300	0.000	1.9
0.4	50 Hz		0.400	0.401	-0.001	1.6
0.5	50 Hz		0.500	0.503	-0.003	1.6
0.6	50 Hz		0.600	0.605	-0.005	2.5
0.7	50 Hz		0.700	0.707	-0.007	2.5
0.3	100 Hz	peak	0.300	0.301	-0.001	1.9
0.4	100 Hz		0.400	0.403	-0.003	1.6
0.5	100 Hz		0.500	0.505	-0.005	1.6
0.6	100 Hz		0.600	0.605	-0.005	2.5
0.7	100 Hz		0.700	0.707	-0.007	2.5

2. VELOCITY RESULT

Test point		Mode	STD Reading	DUC Reading	Correction	Uncertainty
(mm/s)	(frequency)		(mm/s)	(mm/s)	(mm/s)	± (% of rdg.)
3	50 Hz	peak	3.000	3.011	-0.011	1.8
4	50 Hz		4.000	4.030	-0.030	1.8
5	50 Hz		5.000	5.044	-0.044	1.8
6	50 Hz		6.000	6.056	-0.056	1.8
7	50 Hz		7.000	7.079	-0.079	1.8
*3	100 Hz	peak	3.000	3.022	-0.022	1.6
*4	100 Hz		4.000	4.037	-0.037	1.6
*5	100 Hz		5.000	5.041	-0.041	1.6
*6	100 Hz		6.000	6.052	-0.052	1.5
*7	100 Hz		7.000	7.077	-0.077	1.5

Certificate No. Q24128001

F3-011-05/12-23

Page 1 of 4

เอกสารไม่ควบคุม



@clccalibration



CALIBRATION DATA

3. DISPLACEMENT RESULT

Test point		Mode	STD Reading	DUC Reading	Correction	Uncertainty
(mm)	(frequency)		(mm)	(mm)	(mm)	± (% of rdg.)
0.03	50 Hz	peak	0.030	0.030	0.000	2.5
0.04	50 Hz		0.040	0.040	0.000	2.1
0.05	50 Hz		0.050	0.050	0.000	1.9
0.06	50 Hz		0.060	0.061	-0.001	1.8
0.07	50 Hz		0.070	0.071	-0.001	1.8
0.03	100 Hz	peak	0.030	0.030	0.000	2.5
0.04	100 Hz		0.040	0.040	0.000	2.1
0.05	100 Hz		0.050	0.050	0.000	1.9
0.06	100 Hz		0.060	0.061	-0.001	1.8
0.07	100 Hz		0.070	0.071	-0.001	1.8

Note. The Scope of Accredited ANAB Certificate No. ACDM-2814 Version 012 Page 1,2 of 67

* means Calibrations marked " Not ANAB Accredited " in this Certificate have been included for completeness.

This report is valid for the above stated instrument/s only.

End of Certificate

Supplement to Calibration Certificate No. Q24128000

CERTIFICATE OF CALIBRATION

FOR

NOMENCLATURE : VIBRATION METER
MANUFACTURER : INSTANTEL
MODEL / TYPE : 721A2601/721A3301
SERIAL NO. : UM14467/UM14467 [UAE.EFM.096/2562]
CLID. NO. : 252000050
JOB CONTROL NO. : 241203128000
CALIBRATION SERVICE : ☒ IN-LABORATORY ☐ ON-SITE

CUSTOMER : UNITED ANALYST AND ENGINEERING CONSULTANT CO., LTD.

81 SOI UDOMSIK 41, SUKHUMVIT ROAD,
BANGCHAK, PHRAKHANONG, BANGKOK 10260

DATE OF RECEIVED : 03 December 2024

DATE OF ISSUED : 29 January 2025

The report of calibration shall not be reproduced except in full without approval of the Calibration Laboratory Co., Ltd.

Calibrated By :

Approved By :

This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to the International System of Units (SI)

Certificate No. Q24128000A1

F3-012-05/12-23

page 1 of 4

Certificate No. Q24128001

F3-011-05/12-23

page 4 of 4

เอกสารไม่ควบคุม



@clccalibration

เอกสารไม่ควบคุม



@clccalibration



CALIBRATION LABORATORY Co.,LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



CALIBRATION LABORATORY Co.,LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



Supplement to Calibration Certificate No. Q24128000

REPORT OF CALIBRATION

FOR

NOMENCLATURE : VIBRATION METER
MANUFACTURER : INSTANTEL
MODEL / TYPE : 721A2601/721A3301
SERIAL NO. : UM14467/UM14467 [UAE.EFM.096/2562]
DATE OF CALIBRATION : 04 December 2024

ENVIRONMENT CONDITIONS :

Temperature : (23 ± 2) °C Relative Humidity : (55 ± 15) %RH

PROCEDURE USED :

This instrument was calibrated under procedure No. CLC-CPEE-08 based on ISO 16063-21 as calibration guideline.
The calibration was performed by using Digital Multimeter, Programmable Timer/Counter, Vibration Calibrator which maintained by the Calibration Laboratory Co., Ltd.

REFERENCE STANDARD USED :

- Vibration Calibrator, The Modal Shop Model 9110D S/N. 11424.
- Programmable Timer/Counter, Philips Model PM6680B S/N. SM607101.
- Digital Multimeter, Keysight Technologies Model 3458A S/N. MY59352733.

TRACEABILITY :

- The measurements are traceable to International System of Units (SI), through National Institute of Metrology (Thailand) Certificate No. AV-0030-24, Due Date 19 July 2025.
- The measurements are traceable to International System of Units (SI), through Aeronautical Radio of Thailand Ltd. Certificate No. 07-0050/24, Due Date 13 May 2025.
- The measurements are traceable to International System of Units (SI), through National Institute of Metrology (Thailand) Certificate No. EE-0060-24, Due Date 26 June 2025.

UNCERTAINTY :

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor $k = 2$, which for a normal distribution corresponds to a coverage probability of approximately 95 %.

It has been evaluated according to the "Evaluation of the Uncertainty of Measurement in Calibration (EA-4/02 M:2022)"

Certificate No. Q24128000A1
F3-012-05/12-23

page 2 of 4

เอกสารไม่ควบคุม



CALIBRATION LABORATORY Co.,LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



CALIBRATION LABORATORY Co.,LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



CALIBRATION DATA

3. DISPLACEMENT RESULT

Test point		Mode	STD Reading (mm)	DUC Reading (mm)	Correction (mm)	Uncertainty ± (% of rdg.)
(mm)	(frequency)					
0.03	50 Hz	peak	0.030	0.030	0.000	2.5
0.04	50 Hz		0.040	0.040	0.000	2.1
0.05	50 Hz		0.050	0.050	0.000	1.9
0.06	50 Hz		0.060	0.060	0.000	1.8
0.07	50 Hz		0.070	0.071	-0.001	1.8
0.03	100 Hz	peak	0.030	0.030	0.000	2.5
0.04	100 Hz		0.040	0.040	0.000	2.1
0.05	100 Hz		0.050	0.050	0.000	1.9
0.06	100 Hz		0.060	0.060	0.000	1.8
0.07	100 Hz		0.070	0.071	-0.001	1.8

Note. The Scope of Accredited ANAB Certificate No. ACDM-2814 Version 012 Page 1,2 of 67

* means Calibrations marked " Not ANAB Accredited " in this Certificate have been included for completeness.

This report is valid for the above stated instrument/s only.

End of Certificate

Certificate No. Q24128000
F3-011-05/12-23

page 4 of 4

เอกสารไม่ควบคุม



CONDITION OF CALIBRATION ITEM : RECEIVED IN GOOD OPERATIONAL CONDITION

MEASUREMENT RESULTS : (X) without adjustment () adjustment

CALIBRATION DATA

1. ACCELERATION RESULT

Test point		Mode	STD Reading (g)	DUC Reading (g)	Correction (g)	Uncertainty ± (% of rdg.)
(g)	(frequency)					
0.3	50 Hz	peak	0.300	0.302	-0.002	1.9
0.4	50 Hz		0.400	0.402	-0.002	1.6
0.5	50 Hz		0.500	0.503	-0.003	1.6
0.6	50 Hz		0.600	0.603	-0.003	2.5
0.7	50 Hz		0.700	0.705	-0.005	2.5
0.3	100 Hz	peak	0.300	0.301	-0.001	1.9
0.4	100 Hz		0.400	0.402	-0.002	1.6
0.5	100 Hz		0.500	0.502	-0.002	1.6
0.6	100 Hz		0.600	0.603	-0.003	2.5
0.7	100 Hz		0.700	0.705	-0.005	2.5

2. VELOCITY RESULT

Test point		Mode	STD Reading (mm/s)	DUC Reading (mm/s)	Correction (mm/s)	Uncertainty ± (% of rdg.)
(mm/s)	(frequency)					
3	50 Hz	peak	3.000	3.015	-0.015	1.8
4	50 Hz		4.000	4.024	-0.024	1.8
5	50 Hz		5.000	5.034	-0.034	1.8
6	50 Hz		6.000	6.044	-0.044	1.8
7	50 Hz		7.000	7.058	-0.058	1.8
*3	100 Hz	peak	3.000	3.033	-0.033	1.6
*4	100 Hz		4.000	4.047	-0.047	1.6
*5	100 Hz		5.000	5.055	-0.055	1.6
*6	100 Hz		6.000	6.062	-0.062	1.5
*7	100 Hz		7.000	7.080	-0.080	1.5

Certificate No. Q24128000

F3-011-05/12-23

page 3 of 4

เอกสารไม่ควบคุม



CERTIFICATE OF CALIBRATION

FOR

NOMENCLATURE : VIBRATION METER
MANUFACTURER : INSTANTEL
MODEL / TYPE : 721A2601/721A3301
SERIAL NO. : UM14472/UM14472 [UAE.EFM.101/2562]
CLID. NO. : 252000710
JOB CONTROL NO. : 241203127998
CALIBRATION SERVICE : ☒ IN-LABORATORY ☐ ON-SITE

CUSTOMER : UNITED ANALYST AND ENGINEERING CONSULTANT CO., LTD.
81 SOI UDOMSUK 41, SUKHUMVIT ROAD,
BANGCHAK, PHRAKHANONG, BANGKOK 10260

DATE OF RECEIVED : 03 December 2024

DATE OF ISSUED : 29 January 2025

The report of calibration shall not be reproduced except in full without approval of the Calibration Laboratory Co., Ltd.

Calibrated By :

Approved By :

This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to the International System of Units (SI)

Certificate No. Q24127998A1

F3-012-05/12-23

page 1 of 4

เอกสารไม่ควบคุม





CALIBRATION LABORATORY Co.,LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



CALIBRATION LABORATORY Co.,LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



Supplement to Calibration Certificate No. Q24127998

REPORT OF CALIBRATION

FOR

NOMENCLATURE : VIBRATION METER
MANUFACTURER : INSTANTEL
MODEL / TYPE : 721A2601/721A3301
SERIAL NO. : UM14472/UM14472 [UAE.EFM.101/2562]
DATE OF CALIBRATION : 04 December 2024

ENVIRONMENT CONDITIONS :

Temperature : (23 ± 2) °C Relative Humidity : (55 ± 15) %RH

PROCEDURE USED :

This instrument was calibrated under procedure No. CLC-CPEE-08 based on ISO 16063-21 as calibration guideline.
The calibration was performed by using Digital Multimeter, Programmable Timer/Counter, Vibration Calibrator which maintained by the Calibration Laboratory Co., Ltd.

REFERENCE STANDARD USED :

- Vibration Calibrator, The Modal Shop Model 9110D S/N. 11424.
- Programmable Timer/Counter, Philips Model PM6680B S/N. SM607101.
- Digital Multimeter, Keysight Technologies Model 3458A S/N. MY59352733.

TRACEABILITY :

- The measurements are traceable to International System of Units (SI), through National Institute of Metrology (Thailand) Certificate No. AV-0030-24, Due Date 19 July 2025.
- The measurements are traceable to International System of Units (SI), through Aeronautical Radio of Thailand Ltd. Certificate No. 07-0050/24, Due Date 13 May 2025.
- The measurements are traceable to International System of Units (SI), through National Institute of Metrology (Thailand) Certificate No. EE-0060-24, Due Date 26 June 2025.

UNCERTAINTY :

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor $k = 2.00$ which for a normal distribution corresponds to a coverage probability of approximately 95 %.
It has been evaluated according to the "Evaluation of the Uncertainty of Measurement in Calibration (EA-4/02 M:2022)"

Certificate No. Q24127998A1

F3-012-05/12-23

page 2 of 4

เอกสารไม่ควบคุม



@clccalibration

CONDITION OF CALIBRATION ITEM : RECEIVED IN GOOD OPERATIONAL CONDITION

MEASUREMENT RESULTS : (X) without adjustment () adjustment

CALIBRATION DATA

1. ACCELERATION RESULT

Test point		Mode	STD Reading	DUC Reading	Correction	Uncertainty
(g)	(frequency)		(g)	(g)	(g)	± (% of rdg.)
0.3	50 Hz	peak	0.300	0.303	-0.003	1.9
0.4	50 Hz		0.400	0.405	-0.005	1.6
0.5	50 Hz		0.500	0.506	-0.006	1.6
0.6	50 Hz		0.600	0.607	-0.007	2.5
0.7	50 Hz	peak	0.700	0.708	-0.008	2.5
0.3	100 Hz		0.300	0.301	-0.001	1.9
0.4	100 Hz		0.400	0.402	-0.002	1.6
0.5	100 Hz		0.500	0.503	-0.003	1.6
0.6	100 Hz		0.600	0.605	-0.005	2.5
0.7	100 Hz		0.700	0.709	-0.009	2.5

2. VELOCITY RESULT

Test point		Mode	STD Reading	DUC Reading	Correction	Uncertainty
(mm/s)	(frequency)		(mm/s)	(mm/s)	(mm/s)	± (% of rdg.)
3	50 Hz	peak	3.000	3.035	-0.035	1.8
4	50 Hz		4.000	4.042	-0.042	1.8
5	50 Hz		5.000	5.059	-0.059	1.8
6	50 Hz		6.000	6.068	-0.068	1.8
7	50 Hz	peak	7.000	7.086	-0.086	1.8
*3	100 Hz		3.000	3.037	-0.037	1.6
*4	100 Hz		4.000	4.042	-0.042	1.6
*5	100 Hz		5.000	5.057	-0.057	1.6
*6	100 Hz		6.000	6.084	-0.084	1.5
*7	100 Hz		7.000	7.112	-0.112	1.5

Certificate No. Q24127998

F3-011-05/12-23

page 3 of 4

เอกสารไม่ควบคุม



@clccalibration



CALIBRATION LABORATORY Co.,LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7139 MOO 13, SOI SUTINAKORN 11 TAMBON BANG KAO,
AMPHOE BANG PHU SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL: (660) 2116-5800-1 FAX: (660) 2116-7140



Page 1 of 3

CALIBRATION DATA

3. DISPLACEMENT RESULT

Test point		Mode	STD Reading	DUC Reading	Correction	Uncertainty
(mm)	(frequency)		(mm)	(mm)	(mm)	± (% of rdg.)
0.03	50 Hz	peak	0.030	0.030	0.000	2.5
0.04	50 Hz		0.040	0.040	0.000	2.1
0.05	50 Hz		0.050	0.050	0.000	1.9
0.06	50 Hz		0.060	0.061	-0.001	1.8
0.07	50 Hz	peak	0.070	0.071	-0.001	1.8
0.03	100 Hz		0.030	0.030	0.000	2.5
0.04	100 Hz		0.040	0.040	0.000	2.1
0.05	100 Hz		0.050	0.050	0.000	1.9
0.06	100 Hz		0.060	0.061	-0.001	1.8
0.07	100 Hz		0.070	0.071	-0.001	1.8

Note. The Scope of Accredited ANAB Certificate No. ACDM-2814 Version 012 Page 1,2 of 67

* means Calibrations marked " Not ANAB Accredited " in this Certificate have been included for completeness.

This report is valid for the above stated instrument/s only.

End of Certificate

Certificate No. Q24127998

F3-011-05/12-23

page 4 of 4

เอกสารไม่ควบคุม



@clccalibration

Certificate of Calibration

Customer

Name : UNITED ANALYST AND ENGINEERING
CONSULTANT CO.,LTD.
Address : 81 Soi Udomsuk 41, Sukhumvit Road, Bangchak,
Prakanong, Bangkok 10260

Certificate No : 24-ACT-087
Request No : Req-2024-1365

Unit Under Calibration Details

Measurement item : Acoustic Calibrator Class : 1
Manufacturer : 01dB Range : 94 dB / 1000 Hz
Model : CAL31 Instrument Status : Used
Serial Number : 84065
ID : UAE.EFM.167/2561

Calibration Environment and Details

Temperature : (23 ± 2 °C)
Humidity : (50 ± 20 %RH)
Barometric Pressure : (1013 ± 10.0 hPa)
Received Date : 20 June 2024
Calibration Date : 25 June 2024
Location of Calibration : LAB 1 Acoustic
Calibration Procedure : In-house method CP-ACT-02 based on IEC 60942:2017 Electroacoustics - Sound calibrators

Reference Standard	Model	Serial Number	Traceable	Due Calibration
Sound Calibrator	SV 35A	58079	EI	12 June 2025
THD Multimeter	2015	1047765	NIMT	16 January 2025

Traceability : This certificate provides traceability of measurement to recognized national standard, and to the realization of the international System of Units (SI).

Note

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor $k = 2$, providing a level of confidence approximately 95 %.

Calibrated By :



Issue Date : 25 June 2024

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Calibration Laboratory Co., Ltd.

เอกสารไม่ควบคุม

FM-708-ACT-02 Rev 03 Issue date 5/8/24

Certificate No : 24-ACT-087
Request No : Req-2024-1365

Sound pressure level

Calibration Results : Without Adjustment

Calibration Range (dB)	Without Adjustment (dB)		Adjustment (dB)		Uncertainty (± dB)	Acceptance limit Class 1 (± dB)	Result
	Measured	Deviated value	Measured	Deviated value			
94 dB / 1000 Hz	93.78	-0.22	-	-	0.13	0.25	Pass

Frequency of Sound pressure level

Calibration Range (Hz)	Without Adjustment		Adjustment		Uncertainty (± %)	Acceptance limit Class 1 (± %)	Result
	Measured (Hz)	Deviated	Measured (Hz)	Deviated			
94 dB / 1000 Hz	1000.00	0.00	-	-	0.01	0.70	Pass

Total Harmonic Distortion plus Noise of Sound pressure level (THD+N %)

Calibration Range (Hz)	Without Adjustment	Adjustment	Uncertainty (± %)	Acceptance limit Class 1 (± %)	Result
	Measured (%)	Measured (%)			
94 dB / 1000 Hz	0.14	-	0.40	2.5	Pass

Note :

Function	Maximum-permitted Uncertainty of measurement
Sound pressure level	0.15 dB
Frequency	0.20%
Total distortion+noise	0.50%

~ Acceptance limit was IEC60942:2017 Class 1

~ The calibration results exclude the calibrator pressure correction

~ The calibration results exclude the microphone volume correction

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the laboratory.

เอกสารไม่ควบคุม

FM-708-ACT-02 Rev.03 Issue date 5/6/24

Certificate No : 24-ACT-087
Request No : Req-2024-1365

Decision Rule for Statements of Conformity


The standard decision rule employed for the statements of conformity to each calibration result will be applied using ILAC-G8:09:2019: Guidelines on the Reporting of Compliance with Specification as following Fig. and statements

Pass = The measurement result plus the expanded uncertainty with a 95% coverage probability were within the limit.

Pass¹ = The measurement result was within the limit. However, a portion of the expanded uncertainty of measurement at 95% exceeds the limit.

Fail¹ = The measurement result was out of the limit. However, a portion of the expanded uncertainty of measurement at 95% is within the limit.

Fail = The measurement result plus the expanded uncertainty with a 95% coverage probability were outside the limit.

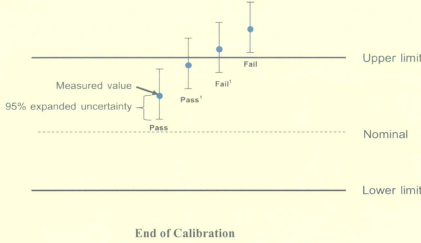

End of Calibration

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the laboratory.

เอกสารไม่ควบคุม

FM-708-ACT-02 Rev.03 Issue date 5/6/24

Page : 1/7.

Certificate of Calibration

Customer

Name : UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.
Address : 81 Soi Udomsuk 41, Sukhumvii Road, Bangchak, Prakanong, Bangkok 10260

Certificate No : 24-SLM-236
Request No : Req-2024-1455

Unit Under Calibration Details

Measurement item : Sound Level Meter
Manufacturer : Larson Davis
Model : LX12
Serial Number : 0006691
ID : UAE.EFM.131/2565
Resolution : 0.1 dB
Microphone Class : 2
Microphone Model : 375A04
Microphone S/N : 335080
Preamplifier Model : PRMLxT2C
Preamplifier S/N : 071565
Instrument Status : Used

Calibration Environment and Details

Temperature : 23 °C ± 2 °C
Humidity : 50 %RH ± 20 %RH
Barometric Pressure : 1013 hPa ± 10 hPa
Received Date : 1 July 2024
Calibrated Date : 10 July 2024
Calibration Procedure : In-house method CP-SLM-01 based on IEC 61672-3 : 2013 Electroacoustics - Sound level meters - Part 3: Periodic tests
Location of Calibration : Lab Acoustic

Reference Standard

Instrument	Brand	Model	SN.	Due calibration	Tracebility
Standard Microphone	GRAS	40AN	188273	20 August 2024	GRAS
Multifrequency Calibrator	Quest	Quest-cal	EFA000234	26 July 2024	TSI
Audio Generator	SvanteK	Svan401	131	8 October 2024	WK Electric

Note
The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor k = 2, providing a level of confidence approximately 95 %.

Issue Date : 10 July 2024

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the laboratory.

เอกสารไม่ควบคุม

FM-708-SLM-01 Rev.04 Issue date 5/6/24

Page : 2/7.

Certificate No : 24-SLM-236
Request No : Req-2024-1455

1. Indication at the calibration check frequency

UUC Setting	Nominal	Before Adjust		After Adjust		UNCERTAINTY	Acceptance	Result
FAST / A / 37-139	Level	UUC	ERR	UUC	ERR			
Calibrator Setting	(dB)	(dB)	(dB)	(dB)	(dB)	(± dB)	Limit (± dB)	
1000 Hz 114 dB	113.76	114.2	0.44	113.8	±0.04	0.20	0.30	Pass

Note : Absolute sensitivity was established by the use of Sound Calibrator Brand SVANTEK, Model SV 35A, SN. 58079

2. Self-generated noise, Microphone installed

UUC Setting FAST / 37-139	Measured (dB)	UNCERTAINTY (± dB)
A	30.9	0.10

3. Self-generated noise, Microphone replaced by the electrical input signal device

UUC Setting FAST / 37-139	Measured (dB)	UNCERTAINTY (± dB)
A	30.8	0.10
C	30.5	0.10
Z	35.0	0.10

4. Acoustic signal test of frequency weightings

(Without Windscreen)

UUC Setting FAST / 37-139 STD Setting	Deviation from various Frequency Weighting Responce curve A C Z (dB) (dB) (dB)			UNCERTAINTY (± dB)	Acceptance Limit (± dB)	Result
	(dB)	(dB)	(dB)			
125 Hz	0.1	0.1	0.1	0.60	1.5	Pass
1000 Hz	0.0	0.0	0.0	0.60	1.0	Pass
4000 Hz	2.0	1.9	1.9	0.60	3.0	Pass
8000 Hz	1.7	1.6	1.7	0.70	5.0	Pass

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the laboratory.

เอกสารไม่ควบคุม

FM-708-SLM-01 Rev.04 Issue date 5/6/24

5. Electrical signal test of frequency weightings, Weighting network response with relative to 1 kHz

UUC Setting	Deviation from various Frequency			UNCERTAINTY	Acceptance	Result
FAST / 37-139	Weighting Resone curve				Limit	
STD Setting	A (dB)	C (dB)	Z (dB)	(± dB)	(± dB)	
63 Hz	-0.1	0.0	0.0	0.20	2.0	Pass
125 Hz	-0.1	0.0	0.0		1.5	Pass
250 Hz	-0.1	0.0	0.0		1.5	Pass
500 Hz	0.0	0.1	0.0		1.5	Pass
1000 Hz	0.0	0.0	0.0		1.0	Pass
2000 Hz	0.0	0.1	0.0		2.0	Pass
4000 Hz	0.0	0.0	0.0		3.0	Pass
8000 Hz	0.0	0.0	0.1		5.0	Pass
16000 Hz	0.0	-0.1	-0.1		+5, -INF.	Pass

6. Frequency and time weightings at 1kHz

UUC Setting	STD	Measured		UNCERTAINTY	Acceptance Limit	Result
		REF	UUC			
FAST / 37-139						
UUC Weighting	(dB)	(dB)	(dB)	(± dB)	(± dB)	
A	114.00	114.0	0.0	0.20	0.20	Pass
C	114.00	114.0	0.0		0.20	Pass
Z	114.00	114.0	0.0		0.20	Pass

UUC Setting	STD	Measured		UNCERTAINTY	Acceptance Limit	Result
		REF	UUC			
37-139 / A						
UUC Time Resone	(dB)	(dB)	(dB)	(± dB)	(± dB)	
Fast	114.00	114.0	0.0	0.20	0.10	Pass1
Slow	114.00	114.0	0.0		0.10	Pass1
Leq	114.00	114.0	0.0		0.10	Pass1

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of **เอกสารไม่ควบคุม**
FM-708-SLM-01 Rev.04 Issue date 5/6/24

7. Long Term Stability

UUC Setting	Measured	UNCERTAINTY	Acceptance Limit	Result
FAST / A / 37-139	UUC			
	(dB)	(± dB)	(± dB)	
STD Setting				
Initial	114.0			
Final	114.0			
Deviated	0.0	0.10	0.30	Pass

8. Level linearity on the reference level range

UUC Setting	Anticipated	Deviation		UNCERTAINTY	Acceptance Limit	Result
		REF	UUC			
FAST / A / 37-139						
STD dB	(dB)	(dB)	(dB)	(± dB)	(± dB)	
139.00	139	139.0	0.0	0.30	1.1	Pass
134.00	134	134.0	0.0		1.1	Pass
129.00	129	129.0	0.0		1.1	Pass
124.00	124	124.0	0.0		1.1	Pass
119.00	119	119.0	0.0		1.1	Pass
114.00	114	114.0	0.0		1.1	Pass
109.00	109	109.0	0.0		1.1	Pass
104.00	104	104.0	0.0		1.1	Pass
99.00	99	99.0	0.0		1.1	Pass
94.00	94	94.0	0.0		1.1	Pass
89.00	89	89.0	0.0		1.1	Pass
84.00	84	84.0	0.0		1.1	Pass
79.00	79	79.0	0.0		1.1	Pass
74.00	74	74.0	0.0		1.1	Pass
69.00	69	69.0	0.0		1.1	Pass
64.00	64	64.0	0.0		1.1	Pass
59.00	59	59.0	0.0		1.1	Pass
54.00	54	54.0	0.0		1.1	Pass
49.00	49	49.1	0.1		1.1	Pass
44.00	44	44.2	0.2		1.1	Pass
43.00	43	43.3	0.3		1.1	Pass
42.00	42	42.3	0.3		1.1	Pass
41.00	41	41.4	0.4		1.1	Pass
40.00	40	40.5	0.5		1.1	Pass

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of **เอกสารไม่ควบคุม**
FM-708-SLM-01 Rev.04 Issue date 5/6/24

9. Level linearity including the level range control

UUC Setting	STD	Measured		UNCERTAINTY	Acceptance Limit	Result
		REF	UUC			
FAST / A						
UUC Range	(dB)	(dB)	(dB)	(± dB)	(± dB)	
37-139	46.00	46.1	0.1	0.30	1.1	Pass
	114	114.0	0.0		1.1	Pass

10. Tone burst response

UUC Setting	STD	Anticipated	Measured		UNCERTAINTY	Acceptance Limit	Result
			Ref	UUC			
A / 37-139							
UUC Time Resone	(ms)	(dB)	(dB)	(dB)	(± dB)	(± dB)	
Fast	200	135.0	135.0	0.0	0.20	1.0	Pass
	2	118.0	117.8	-0.2		+1.0, -2.5	Pass
	0.25	109.0	108.5	-0.5		+1.5, -5.0	Pass
Slow	200	128.6	128.5	-0.1		1.0	Pass
	2	109.0	108.8	-0.2		+1.0, -5.0	Pass
	200	129.0	129.0	0.0		1.0	Pass
SEL	2	109.0	109.0	0.0		+1.0, -2.5	Pass
	0.25	100.0	99.7	-0.3		+1.5, -5.0	Pass

11. Peak C Sound level

UUC Setting	Anticipated	Measured		UNCERTAINTY	Acceptance Limit	Result
		REF	UUC			
FAST / C / 95-142						
STD Setting	(dB)	(dB)	(dB)	(± dB)	(± dB)	
Complete cycle	137.4	136.6	-0.80	0.20	3.0	Pass
Positive half cycle	136.4	136.2	-0.20		2.0	Pass
Negative half cycle	136.4	136.2	-0.20		2.0	Pass

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of **เอกสารไม่ควบคุม**
FM-708-SLM-01 Rev.04 Issue date 5/6/24

12. Overload indication

UUC Setting	Measured	UNCERTAINTY	Acceptance Limit	Result
FAST / A / 37-139	UUC			
	(dB)	(± dB)	(± dB)	
STD Setting				
Positive one-half cycle	144.9			
Negative one-half cycle	144.9			
Deviated	0.0	0.20	1.5	Pass

13. High Level Stability


UUC Setting	Measured	UNCERTAINTY	Acceptance Limit	Result
FAST / A / 37-139	UUC			
	(dB)	(± dB)	(± dB)	
STD Setting				
Initial	138.0			
Final	138.0			
Deviated	0.0	0.10	0.30	Pass

Note :

Function	Maximum-permitted Uncertainty of measurement
1. Indication at the calibration check frequency	Not applicable
2. Self-generated noise, Microphone installed	Not applicable
3. Self-generated noise, Microphone replaced by the electrical input signal device	Not applicable
4. Acoustic signal test of frequency weightings at 10 Hz to 4 kHz	0.60 dB
4. Acoustic signal test of frequency weightings at >4 kHz to 10 kHz	0.70 dB
5. Electrical signal test of frequency weightings, Weighting network response with relative to 1 kHz	0.20 dB
6. Frequency and time weightings at 1kHz	0.20 dB
7. Long Term Stability	0.10 dB
8. Level linearity on the reference level range	0.30 dB
9. Level linearity including the level range control	0.30 dB
10. Tone burst response	0.30 dB
11. Peak C Sound level	0.35 dB
12. Overload indication	0.25 dB
13. High Level Stability	0.10 dB

- Acceptance limit and Maximum-permitted Uncertainty was IEC 61672-1:2013

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of **เอกสารไม่ควบคุม**
FM-708-SLM-01 Rev.04 Issue date 5/6/24

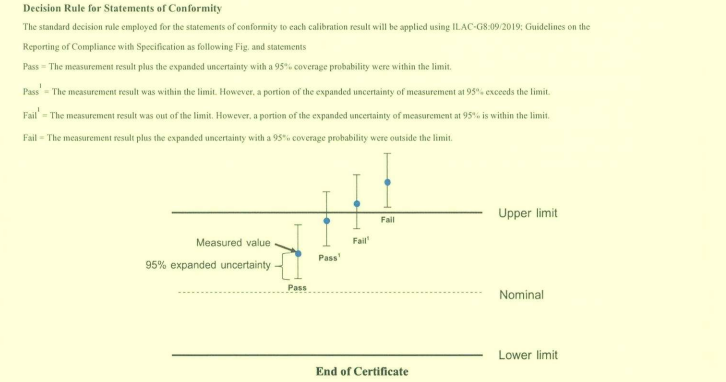

Customer

Name

: UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.

Address

: 81 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Prakanong, Bangkok 10260

Certificate No : 24-SLM-229

Request No : Req-2024-1448

Unit Under Calibration Details

Measurement item : Sound Level Meter

Manufacturer : Larson Davis

Model : LxT2

Serial Number : 0005372

ID : UAE.EFM.037/2563

Resolution : 0.1 dB

Microphone Class : 2

Microphone Model : 375B02

Microphone S/N : 11792

Preamplifier Model : PRMLXT2B

Preamplifier S/N : 056132

Instrument Status : Used

Calibration Environment and Details

Temperature : 23 °C ± 2 °C

Humidity : 50 %RH ± 20 %RH

Barometric Pressure : 1013 hPa ± 10 hPa

Received Date : 1 July 2024

Calibrated Date : 9 July 2024

Calibration Procedure : In-house method CP-SLM-01 based on IEC 61672-3 : 2013 Electroacoustics - Sound level meters - Part 3: Periodic tests

Location of Calibration : Lab Acoustic

Reference Standard

Instrument	Brand	Model	SN.	Due calibration	Tracebility
Standard Microphone	GRAS	40AN	188273	20 August 2024	GRAS
Multifrequency Calibrator	Quest	Quest-cal	EFA000234	26 July 2024	TSI
Audio Generator	Svantek	Svan401	131	8 October 2024	WK Electric

Note

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor $k = 2$, providing a level of confidence approximately 95 %.



1. Indication at the calibration check frequency

UUC Setting	Nominal	Before Adjust		After Adjust		UNCERTAINTY (± dB)	Acceptance Limit (± dB)	Result
	Level	UUC	ERR	UUC	ERR			
Calibrator Setting	(dB)	(dB)	(dB)	(dB)	(dB)			
1000 Hz 114 dB	113.76	114.7	0.94	113.8	+0.04	0.20	0.30	Pass

Note : Absolute sensitivity was established by the use of Sound Calibrator Brand SVANTEK, Model SV 35A, SN. 58079

2. Self-generated noise, Microphone installed

UUC Setting	Measured	UNCERTAINTY
FAST / 37-139		
UUC Weighting	(dB)	(± dB)
A	32.0	0.10

3. Self-generated noise, Microphone replaced by the electrical input signal device

UUC Setting	Measured	UNCERTAINTY
FAST / 37-139		
UUC Weighting	(dB)	(± dB)
A	31.8	0.10
C	31.7	0.10
Z	35.0	0.10

4. Acoustic signal test of frequency weightings (Without Windscreen)

UUC Setting	Deviation from various Frequency Weighting Responce curve			UNCERTAINTY (± dB)	Acceptance Limit (± dB)	Result
	A	C	Z			
FAST / 37-139	(dB)	(dB)	(dB)	0.60	1.5	Pass
STD Setting	(dB)	(dB)	(dB)			
125 Hz	0.1	0.2	0.1			
1000 Hz	0.0	0.0	0.0			
4000 Hz	0.3	0.3	0.4			
8000 Hz	0.3	0.3	0.5	0.70	5.0	Pass

5. Electrical signal test of frequency weightings, Weighting network responce with relative to 1 kHz

UUC Setting	Deviation from various Frequency Weighting Responce curve			UNCERTAINTY (± dB)	Acceptance Limit (± dB)	Result
FAST / 37-139	A (dB)	C (dB)	Z (dB)			
STD Setting	(dB)	(dB)	(dB)	0.20	2.0	Pass
63 Hz	-0.1	0.0	0.0			
125 Hz	-0.1	0.0	0.0			
250 Hz	-0.1	0.0	0.0			
500 Hz	0.0	0.0	0.0			
1000 Hz	0.0	0.0	0.0			
2000 Hz	0.0	0.1	0.0			
4000 Hz	0.0	0.0	0.0			
8000 Hz	0.0	0.0	0.1			
16000 Hz	0.0	0.0	0.0		+5, -INF.	Pass

6. Frequency and time weightings at 1kHz

UUC Setting	STD	Measured		UNCERTAINTY (± dB)	Acceptance Limit (± dB)	Result
FAST / 37-139	REF	UUC	ERR			
UUC Weighting	(dB)	(dB)	(dB)	0.20	0.20	Pass
A	114.00	114.0	0.0			
C	114.00	114.0	0.0			
Z	114.00	114.0	0.0			

UUC Setting	STD	Measured		UNCERTAINTY (± dB)	Acceptance Limit (± dB)	Result
37-139 / A	REF	UUC	ERR			
UUC Time Responce	(dB)	(dB)	(dB)	0.20	0.10	PassI
Fast	114.00	114.0	0.0			
Slow	114.00	114.0	0.0			
Leq	114.00	114.0	0.0			

Certificate No : 24-SLM-229
Request No : Req-2024-1448

7. Long Term Stability

UUC Setting	Measured	UNCERTAINTY	Acceptance	Result
FAST / A / 37-139	UUC	(± dB)	(± dB)	
STD Setting	(dB)			
Initial	114.0			
Final	114.0			
Deviated	0.0	0.10	0.30	Pass

8. Level linearity on the reference level range

UUC Setting	Anticipated	Deviation	UNCERTAINTY	Acceptance	Result
FAST / A / 37-139	REF	UUC	ERR	Limit	Result
STD dB	(dB)	(dB)	(dB)	(± dB)	(± dB)
139.00	139	139.0	0.0	1.1	Pass
134.00	134	134.0	0.0	1.1	Pass
129.00	129	129.0	0.0	1.1	Pass
124.00	124	124.0	0.0	1.1	Pass
119.00	119	119.0	0.0	1.1	Pass
114.00	114	114.0	0.0	1.1	Pass
109.00	109	109.0	0.0	1.1	Pass
104.00	104	104.0	0.0	1.1	Pass
99.00	99	99.0	0.0	1.1	Pass
94.00	94	93.6	-0.4	1.1	Pass
89.00	89	88.6	-0.4	1.1	Pass
84.00	84	83.6	-0.4	1.1	Pass
79.00	79	78.6	-0.4	1.1	Pass
74.00	74	73.6	-0.4	1.1	Pass
69.00	69	68.6	-0.4	1.1	Pass
64.00	64	63.6	-0.4	1.1	Pass
59.00	59	58.6	-0.4	1.1	Pass
54.00	54	53.6	-0.4	1.1	Pass
49.00	49	48.7	-0.3	1.1	Pass
44.00	44	43.9	-0.1	1.1	Pass
39.00	39	39.5	0.5	1.1	Pass
34.00	34	34.9	0.9	1.1	Pass

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of **เอกสารไม่ควบคุม**
FM-708-SLM-01 Rev.04 Issue date 5/6/24

Certificate No : 24-SLM-229
Request No : Req-2024-1448

9. Level linearity including the level range control

UUC Setting	STD	Measured	UNCERTAINTY	Acceptance	Result
FAST / A	REF	UUC	ERR	Limit	Result
UUC Range	(dB)	(dB)	(dB)	(± dB)	(± dB)
37-139	39.10	39.6	0.5	1.1	Pass
	114	114.0	0.0	1.1	Pass

10. Tone burst response

UUC Setting	STD	Anticipated	Measured	UNCERTAINTY	Acceptance	Result
A / 37-139	Toneburst	Ref	UUC	ERR	Limit	Result
UUC Time Response	(ms)	(dB)	(dB)	(dB)	(± dB)	(± dB)
Fast	200	135.0	135.0	0.0	1.0	Pass
	2	118.0	117.9	-0.1	+1.0, -2.5	Pass
	0.25	109.0	108.8	-0.2	+1.5, -5.0	Pass
Slow	200	128.6	128.5	-0.1	1.0	Pass
	2	109.0	108.9	-0.1	+1.0, -5.0	Pass
SEL	200	129.0	129.0	0.0	1.0	Pass
	2	109.0	109.1	+0.1	+1.0, -2.5	Pass
	0.25	100.0	100.0	0.0	+1.5, -5.0	Pass

11. Peak C Sound level

UUC Setting	Anticipated	Measured	UNCERTAINTY	Acceptance	Result
FAST / C / 95-142	REF	UUC	ERR	Limit	Result
STD Setting	(dB)	(dB)	(dB)	(± dB)	(± dB)
Complete cycle	137.4	136.8	-0.60	3.0	Pass
Positive half cycle	136.4	136.2	-0.20	2.0	Pass
Negative half cycle	136.4	136.2	-0.20	2.0	Pass

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of **เอกสารไม่ควบคุม**
FM-708-SLM-01 Rev.04 Issue date 5/6/24

Certificate No : 24-SLM-229
Request No : Req-2024-1448

12. Overload indication

UUC Setting	Measured	UNCERTAINTY	Acceptance	Result
FAST / A / 37-139	UUC	(± dB)	(± dB)	
STD Setting	(dB)			
Positive one-half cycle	140.7			
Negative one-half cycle	140.7			
Deviated	0.0	0.20	1.5	Pass

13. High Level Stability

UUC Setting	Measured	UNCERTAINTY	Acceptance	Result
FAST / A / 37-139	UUC	(± dB)	(± dB)	
STD Setting	(dB)			
Initial	138.0			
Final	138.0			
Deviated	0.0	0.10	0.30	Pass

Note :

Function	Maximum-permitted Uncertainty of measurement
1. Indication at the calibration check frequency	Not applicable
2. Self-generated noise, Microphone installed	Not applicable
3. Self-generated noise, Microphone replaced by the electrical input signal device	Not applicable
4. Acoustic signal test of frequency weightings at 10 Hz to 4 kHz	0.60 dB
4. Acoustic signal test of frequency weightings at >4 kHz to 10 kHz	0.70 dB
5. Electrical signal test of frequency weightings, Weighting network response with relative to 1 kHz	0.20 dB
6. Frequency and time weightings at 1kHz	0.20 dB
7. Long Term Stability	0.10 dB
8. Level linearity on the reference level range	0.30 dB
9. Level linearity including the level range control	0.30 dB
10. Tone burst response	0.30 dB
11. Peak C Sound level	0.35 dB
12. Overload indication	0.25 dB
13. High Level Stability	0.10 dB

- Acceptance limit and Maximum-permitted Uncertainty was IEC 61672-1:2013

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of **เอกสารไม่ควบคุม**
FM-708-SLM-01 Rev.04 Issue date 5/6/24

Certificate No : 24-SLM-229
Request No : Req-2024-1448

Decision Rule for Statements of Conformity


The standard decision rule employed for the statements of conformity to each calibration result will be applied using ILAC-G8:09/2019: Guidelines on the Reporting of Compliance with Specification as following Fig, and statements

Pass = The measurement result plus the expanded uncertainty with a 95% coverage probability were within the limit.

Pass¹ = The measurement result was within the limit. However, a portion of the expanded uncertainty of measurement at 95% exceeds the limit.

Fail¹ = The measurement result was out of the limit. However, a portion of the expanded uncertainty of measurement at 95% is within the limit.

Fail = The measurement result plus the expanded uncertainty with a 95% coverage probability were outside the limit.

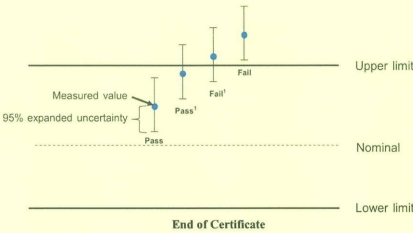

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of **เอกสารไม่ควบคุม**
FM-708-SLM-01 Rev.04 Issue date 5/6/24



Certificate of Calibration

Customer

Name : UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.
Address : 81 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Prakanong, Bangkok 10260

Certificate No : 24-SLM-239
Request No : Req-2024-1458

Unit Under Calibration Details

Measurement item : Sound Level Meter
Manufacturer : Larson Davis
Model : LxT2
Serial Number : 0006756
ID : UAE-EFM.032/2566
Resolution : 0.1 dB
Microphone Class : 2
Microphone Model : 375A04
Microphone S/N : 346384
Preamplifier Model : PRMLXTC2
Preamplifier S/N : 073885
Instrument Status : Used

Calibration Environment and Details

Temperature : 23 °C ± 2 °C
Humidity : 50 %RH ± 20 %RH
Barometric Pressure : 1013 hPa ± 10 hPa
Received Date : 2 July 2024
Calibrated Date : 11 July 2024
Calibration Procedure : In-house method CP-SLM-01 based on IEC 61672-3 : 2013 Electroacoustics - Sound level meters - Part 3: Periodic tests
Location of Calibration : Lab Acoustic

Reference Standard

Instrument	Brand	Model	SN	Due calibration	Traceability
Standard Microphone	GRAS	40AN	188273	20 August 2024	GRAS
Multifrequency Calibrator	Quest	Quest-cal	EFA000234	26 July 2024	TSI
Audio Generator	SvanteK	Svan401	131	8 October 2024	WK Electric

Note
The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor $k = 2$, providing a level of confidence approximately 95 %.



Issue Date : 11 July 2024

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the owner.
เอกสารไม่ควบบน
FM-708-SLM-01 Rev.04 Issn: date 5/6/24



Certificate No : 24-SLM-239
Request No : Req-2024-1458

1. Indication at the calibration check frequency

UUC Setting	Nominal	Before Adjust		After Adjust		UNCERTAINTY (± dB)	Acceptance Limit (± dB)	Result
FAST / A / 37-139	Level	UUC (dB)	ERR (dB)	UUC (dB)	ERR (dB)			
1000 Hz 114 dB	113.76	115.1	1.34	113.8	+0.04	0.20	0.30	Pass

Note : Absolute sensitivity was established by the use of Sound Calibrator Brand SVANTEK, Model SV 35A, SN. 58079

2. Self-generated noise, Microphone installed

UUC Setting	Measured	UNCERTAINTY
FAST / 37-139		
UUC Weighting	(dB)	(± dB)
A	27.5	0.10

3. Self-generated noise, Microphone replaced by the electrical input signal device

UUC Setting	Measured	UNCERTAINTY
FAST / 37-139		
UUC Weighting	(dB)	(± dB)
A	27.3	0.10
C	26.8	0.10
Z	31.0	0.10

4. Acoustic signal test of frequency weightings (Without Windscreen)

UUC Setting	Deviation from various Frequency Weighting Responce curve			UNCERTAINTY (± dB)	Acceptance Limit (± dB)	Result
	A (dB)	C (dB)	Z (dB)			
FAST / 37-139						
STD Setting	(dB)	(dB)	(dB)			
125 Hz	0.1	0.2	0.2	0.60	1.5	Pass
1000 Hz	0.0	0.0	0.0	0.60	1.0	Pass
4000 Hz	-0.7	-0.7	-0.7	0.60	3.0	Pass
8000 Hz	-1.7	-1.7	-1.6	0.70	5.0	Pass

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the owner.
เอกสารไม่ควบบน
FM-708-SLM-01 Rev.04 Issn: date 5/6/24



Certificate No : 24-SLM-239
Request No : Req-2024-1458

5. Electrical signal test of frequency weightings, Weighting network response with relative to 1 kHz

UUC Setting	Deviation from various Frequency Weighting Responce curve			UNCERTAINTY (± dB)	Acceptance Limit (± dB)	Result
	A (dB)	C (dB)	Z (dB)			
FAST / 37-139						
STD Setting	(dB)	(dB)	(dB)			
63 Hz	-0.2	-0.1	-0.1	0.20	2.0	Pass
125 Hz	-0.1	0.0	-0.1		1.5	Pass
250 Hz	-0.1	0.0	-0.1		1.5	Pass
500 Hz	-0.1	0.0	-0.1		1.5	Pass
1000 Hz	0.0	0.0	-0.1		1.0	Pass
2000 Hz	0.0	0.0	0.0		2.0	Pass
4000 Hz	0.0	0.0	0.0		3.0	Pass
8000 Hz	-0.1	-0.1	0.0		5.0	Pass
16000 Hz	-0.1	-0.1	-0.1		+5,-INF.	Pass

6. Frequency and time weightings at 1kHz

UUC Setting	STD	Measured		UNCERTAINTY (± dB)	Acceptance Limit (± dB)	Result
FAST / 37-139	REF	UUC	ERR			
UUC Weighting	(dB)	(dB)	(dB)	0.20	0.20	Pass
A	114.00	114.0	0.0			
C	114.00	114.0	0.0			
Z	114.00	114.0	0.0			

UUC Setting	STD	Measured		UNCERTAINTY (± dB)	Acceptance Limit (± dB)	Result
37-139 / A	REF	UUC	ERR			
UUC Time Responce	(dB)	(dB)	(dB)	0.20	0.10	Pass
Fast	114.00	114.0	0.0			
Slow	114.00	114.0	0.0			
Leq	114.00	114.0	0.0			

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the owner.
เอกสารไม่ควบบน
FM-708-SLM-01 Rev.04 Issn: date 5/6/24



Certificate No : 24-SLM-239
Request No : Req-2024-1458

7. Long Term Stability

UUC Setting	Measured	UNCERTAINTY (± dB)	Acceptance Limit (± dB)	Result
FAST / A / 37-139	UUC			
STD Setting	(dB)	0.10	0.30	Pass
Initial	114.0			
Final	114.0			
Deviated	0.0			

8. Level linearity on the reference level range

UUC Setting	Anticipated	Deviation		UNCERTAINTY (± dB)	Acceptance Limit (± dB)	Result
FAST / A / 37-139	REF	UUC	ERR			
STD dB	(dB)	(dB)	(dB)	0.30	1.1	Pass
139.00	139	139.0	0.0			
134.00	134	134.0	0.0			
129.00	129	129.0	0.0			
124.00	124	124.0	0.0			
119.00	119	119.0	0.0			
114.00	114	114.0	0.0			
109.00	109	109.0	0.0			
104.00	104	104.0	0.0			
99.00	99	99.0	0.0			
94.00	94	93.9	-0.1			
89.00	89	88.9	-0.1			
84.00	84	83.9	-0.1			
79.00	79	78.9	-0.1			
74.00	74	73.9	-0.1			
69.00	69	68.9	-0.1			
64.00	64	63.9	-0.1			
59.00	59	58.9	-0.1			
54.00	54	53.9	-0.1			
49.00	49	49.0	0.0			
44.00	44	44.0	0.0			
39.00	39	39.3	0.3			
38.00	38	38.3	0.3			
37.00	37	37.4	0.4			

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the owner.
เอกสารไม่ควบบน
FM-708-SLM-01 Rev.04 Issn: date 5/6/24



Certificate No : 24-SLM-239
Request No : Req-2024-1458

Certificate No : 24-SLM-239
Request No : Req-2024-1458

9. Level linearity including the level range control

UUC Setting	STD	Measured		UNCERTAINTY (± dB)	Acceptance Limit	Result
FAST / A	REF	UUC	ERR		± dB	
UUC Range	(dB)	(dB)	(dB)			
37-139	42.50	42.6	0.1	0.30	1.1	Pass
	114	114.0	0.0		1.1	Pass

10. Tone burst response

UUC Setting	STD	Anticipated	Measured		UNCERTAINTY (± dB)	Acceptance	Result
A / 37-139	Toneburst	Ref	UUC	ERR		Limit	
UUC Time Response	(ms)	(dB)	(dB)	(dB)		(± dB)	
Fast	200	135.0	135.0	0.0	0.20	1.0	Pass
	2	118.0	117.8	-0.2		+1.0, -2.5	Pass
	0.25	109.0	108.6	-0.4		+1.5, -5.0	Pass
Slow	200	128.6	128.5	-0.1		1.0	Pass
	2	109.0	108.9	-0.1		+1.0, -5.0	Pass
	200	129.0	129.0	0.0		1.0	Pass
SEL	2	109.0	109.0	0.0		+1.0, -2.5	Pass
	0.25	100.0	99.8	-0.2		+1.5, -5.0	Pass

11. Peak C Sound level

UUC Setting	Anticipated	Measured		UNCERTAINTY (± dB)	Acceptance	Result
FAST / C / 95-142	REF	UUC	ERR		Limit	
STD Setting	(dB)	(dB)	(dB)		(± dB)	
Complete cycle	137.4	136.7	-0.70	0.20	3.0	Pass
Positive half cycle	136.4	136.2	-0.20		2.0	Pass
Negative half cycle	136.4	136.2	-0.20		2.0	Pass

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the

เอกสารไม่ควบคุม

FM-708-SLM-01 Rev.04 Issue date 5/6/24

12. Overload indication

UUC Setting	Measured	UNCERTAINTY (± dB)	Acceptance	Result
FAST / A / 37-139	UUC		Limit	
STD Setting	(dB)		(± dB)	
Positive one-half cycle	141.3			
Negative one-half cycle	141.2			
Deviated	0.1			
		0.20	1.5	Pass

13. High Level Stability

UUC Setting	Measured	UNCERTAINTY (± dB)	Acceptance Limit	Result
FAST / A / 37-139	UUC		(± dB)	
STD Setting	(dB)		(± dB)	
Initial	138.0			
Final	138.0			
Deviated	0.0	0.10	0.30	Pass

Note :

Function	Maximum-permitted Uncertainty of measurement
1. Indication at the calibration check frequency	Not applicable
2. Self-generated noise, Microphone installed	Not applicable
3. Self-generated noise, Microphone replaced by the electrical input signal device	Not applicable
4. Acoustic signal test of frequency weightings at 10 Hz to 4 kHz	0.60 dB
4. Acoustic signal test of frequency weightings at >4 kHz to 10 kHz	0.70 dB
5. Electrical signal test of frequency weightings, Weighting network response with relative to 1 kHz	0.20 dB
6. Frequency and time weightings at 1kHz	0.20 dB
7. Long Term Stability	0.10 dB
8. Level linearity on the reference level range	0.30 dB
9. Level linearity including the level range control	0.30 dB
10. Tone burst response	0.30 dB
11. Peak C Sound level	0.35 dB
12. Overload indication	0.25 dB
13. High Level Stability	0.10 dB

- Acceptance limit and Maximum-permitted Uncertainty was IEC 61672-1:2013

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the

เอกสารไม่ควบคุม

FM-708-SLM-01 Rev.04 Issue date 5/6/24



Certificate No : 24-SLM-239
Request No : Req-2024-1458

Decision Rule for Statements of Conformity


The standard decision rule employed for the statements of conformity to each calibration result will be applied using ILAC-G8:09/2019: Guidelines on the Reporting of Compliance with Specification as following Fig. and statements

Pass = The measurement result plus the expanded uncertainty with a 95% coverage probability were within the limit.

Pass¹ = The measurement result was within the limit. However, a portion of the expanded uncertainty of measurement at 95% exceeds the limit.

Fail¹ = The measurement result was out of the limit. However, a portion of the expanded uncertainty of measurement at 95% is within the limit.

Fail = The measurement result plus the expanded uncertainty with a 95% coverage probability were outside the limit.

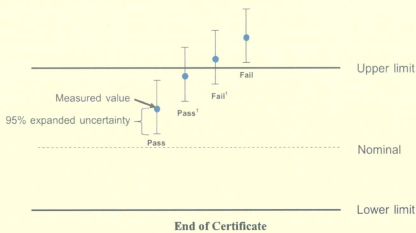

End of Certificate

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the

เอกสารไม่ควบคุม

FM-708-SLM-01 Rev.04 Issue date 5/6/24



ELECTRICAL AND ELECTRONICS INSTITUTE
FOUNDATION FOR INDUSTRIAL DEVELOPMENT
975 Moo 4, Bangpoo Industrial Estate, Soi 8, Sukhumvit Road km 37,
Phraek Sa, Mueang Samut Prakan, Samut Prakan 10280
Tel: +66 2709 4860 Fax: +66 2324 0917



Certificate No.: CP20240321EA
Operation No.: CP2024080292

Certificate of Calibration

Equipment: Sound Level Meter
Manufacturer: Larson Davis (Meter), PCB (Microphone), PCB (Preamplifier)
Model/Type: LxT2 (Meter), 375A04 (Microphone), PRLxT2C (Preamplifier)
Serial No.: 0006757 (Meter), 350420 (Microphone), 073886 (Preamplifier)
ID No.: UAE.EFM.033/2566
Customer: United Analyst and Engineering Consultant Co.,Ltd.
Address: 81 Soi Udumsuk 41, Sukhumvit Road, Bangchak Phrakhanong, Bangkok 10260
Received Date: 9 August 2024
Calibrated Date: 22 - 26 August 2024
Issued Date: 28 August 2024

This report was prepared electronically using applicable electronic signature. Printing or copy of file are considered as a copy of the document.
The reported uncertainty of measurement was based on standard uncertainty multiplied by a coverage factor (k) providing a level of confidence of approximately 95%. This certificate may not be reproduced other than in full except with the prior written approval of the Electrical and Electronics Institute, Foundation for Industrial Development.

เอกสารไม่ควบคุม

Certificate No.: CP20240321EA

Calibration Report

Equipment: Sound Level Meter
Manufacturer: Larson Davis (Meter), PCB (Microphone), PCB (Preamplifier)
Model/Type: LxT2 (Meter), 375A04 (Microphone), PRLMT2C (Preamplifier)
Serial No.: 0006757 (Meter), 350420 (Microphone), 073886 (Preamplifier)
ID No.: UAE EFM.033/2566
Ambient Temperature: (23 ± 2) °C
Relative Humidity: (50 ± 15) %
Pressure: (101.3 ± 1.5) kPa

Method of Calibration :-
IEC 61672-3:2013.

Condition of this result of calibration

1. Reference standards instrument :-

	Instrument	Model	Serial No.	Cert. No.	Due Date
1)	Standard microphone	4180	2787490	AA-1012-23	12 November 2024
2)	Arbitrary Function Generator	AFG2021	C010063	CK20240048EA	23 June 2025
3)	Programmable Attenuator	PA5	2755	EF-0040-23	1 October 2024
4)	6.5 Digit precision multimeter	8846A	9610014	CB20230200EA	15 November 2024
5)	Pressure humidity and Temperature Transmitter	PTU301	L3950483	CL1-P240023 CD20240142EA	24 March 2025 12 June 2025
6)	Pressure humidity and Temperature Transmitter	PTU301	L3950484	CL1-P240030 CD20240143EA	11 April 2025 12 June 2025
7)	Performance Audio Analyzer	U8903B	MY56510003	CB20240035EB CK20230072EA	13 February 2025 13 September 2024

2. This result of calibration was found accurate as shown on date and place of calibration only.

3. This certification is traceable to the international system of unit maintained at :-

Reference standards instrument for Acoustic function

- National Institute of Metrology (Thailand)

Reference standards instrument for Electrical function

- National Institute of Metrology (Thailand)

- Electrical and Electronics Institute; NSC Accredited Calibration No.0119

Result of Calibration:-

Function : 1. Indication at the calibration check frequency

Reference Acoustic Signal (dB)	Measured value (dB)	Deviation (dB)	Acceptance limits (dB)
-	-	-	-

เอกสารไม่ควบคุม

Page 2 of 6

F-CAL-005 Ed.1

Certificate No.: CP20240321EA

Calibration Report

5.2 Time weighting at 1 kHz

Time Weighting	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
Fast	94.0	0.0	±0.1
Slow	94.0	0.0	±0.1
LAeq	94.0	0.0	±0.1

Function : 6. Long-Term Stability

Long-term stability over 30 minutes, with steady 1 kHz signal at reference level.

Time Period to Apply Signal (min)	Reference SPL (dB)	Record SPL at Conclusion of Time Period (dB)	Deviated value (dB)	Acceptance limits (dB)
30	94.0	94.0	0.0	±0.3

Function : 7. Level Linearity on the reference level range

7.1 Level Linearity on the reference level range, Upper

Anticipated Value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
94.0	94.0	0.0	±1.1
99.0	99.0	0.0	±1.1
104.0	104.0	0.0	±1.1
109.0	109.0	0.0	±1.1
114.0	114.0	0.0	±1.1
119.0	119.0	0.0	±1.1
124.0	124.0	0.0	±1.1
129.0	129.0	0.0	±1.1
134.0	134.1	0.1	±1.1
139.0	139.1	0.1	±1.1

เอกสารไม่ควบคุม

Page 4 of 6

F-CAL-005 Ed.1

Certificate No.: CP20240321EA

Calibration Report

Function : 2. Self-generated Noise

2.1 Microphone Installed

Measured value (dB)
28.4

2.2 Microphone replaced by the electrical input signal device

Frequency Weighting	Measured value (dB)
A-weighting	28.2
C-weighting	28.0
Z-weighting	33.3

Function : 3. Acoustical signal tests of frequency weightings (Without Windscreen)

Meter free-field acoustic response at a level of 84 dB.

Frequency (Hz)	Deviation from various Frequency Weighting Response Curve			
	C-Weighting (dB)	A-Weighting (dB)	Z-Weighting (dB)	Acceptance limits (dB)
125	0.1	0.0	0.1	±1.5
1000	0.0	0.0	0.0	±1.0
8000	-0.4	-0.3	-0.2	±5.0

Function : 4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various Frequency Weighting Response Curve			
	C-Weighting (dB)	A-Weighting (dB)	Z-Weighting (dB)	Acceptance limits (dB)
63	0.0	0.0	0.0	±2.0
125	0.0	-0.1	0.0	±1.5
250	0.0	-0.1	0.0	±1.5
500	0.0	-0.1	0.0	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.0	0.0	±2.0
4000	0.0	0.0	0.0	±3.0
8000	-0.1	0.0	0.1	±5.0

Function : 5. Frequency and time weighting at 1 kHz

5.1 Frequency weighting at 1 kHz

Frequency Weighting	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
C-weighting	94.0	0.0	±0.2
A-weighting	94.0	0.0	±0.2
Z-weighting	94.0	0.0	±0.2

เอกสารไม่ควบคุม

Page 3 of 6

F-CAL-005 Ed.1

Certificate No.: CP20240321EA

Calibration Report

7.2 Level Linearity on the reference level range, Lower

Anticipated Value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
94.0	94.0	0.0	±1.1
89.0	89.0	0.0	±1.1
84.0	84.0	0.0	±1.1
79.0	79.0	0.0	±1.1
74.0	74.0	0.0	±1.1
69.0	69.0	0.0	±1.1
64.0	64.0	0.0	±1.1
59.0	59.0	0.0	±1.1
54.0	54.0	0.0	±1.1
49.0	49.0	0.0	±1.1
44.0	44.1	0.1	±1.1
43.0	43.1	0.1	±1.1
42.0	42.1	0.1	±1.1
41.0	41.1	0.1	±1.1
40.0	40.1	0.1	±1.1
39.0	39.3	0.3	±1.1

Function : 8. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
Fast	200	136.0	0.0	±1.0
	2	118.8	-0.2	+1.0 ; -2.5
	0.25	109.8	-0.2	+1.5 ; -5.0
Slow	200	129.5	-0.1	±1.0
	2	109.9	-0.1	+1.0 ; -5.0
	200	130.0	0.0	±1.0
LAE	2	110.0	0.0	+1.0 ; -2.5
	0.25	101.0	0.0	+1.5 ; -5.0

Function : 9. Peak C sound level

Number of cycles in test signal	Anticipated Value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
Complete cycle	135.4	134.7	-0.7	±3.0
Positive half cycle	134.4	134.0	-0.4	±2.0
Negative half cycle	134.4	134.0	-0.4	±2.0

Function : 10. Overload indication

Measured value (dB)		Deviated value (dB)	Acceptance limits (dB)
Positive one-half cycle	Negative one-half cycle		
142.3	142.2	-0.1	±0.1

เอกสารไม่ควบคุม

Page 5 of 6

F-CAL-005 Ed.1

Certificate No.: CP20240321EA

Calibration Report

Function : 11. High-Level Stability

High-Level stability over 5 minutes, with steady 1 kHz signal, 1 dB below upper boundary.

Time Period to Apply Signal (min)	Reference SPL (dB)	Record SPL at Conclusion of Time Period (dB)	Deviated value (dB)	Acceptance limits (dB)
5	139.0	139.0	0.0	±0.3

Uncertainty of measurement

Function	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1) Indication at the calibration check frequency	0.30	Not applicable
2) Self-generated Noise	0.10	Not applicable
3) Acoustical signal tests of frequency weightings - Free-field sound pressure response level	0.30	0.60 (10Hz to 4kHz) 0.70 (>4kHz to 10kHz)
4) Electrical signal tests of frequency weightings	0.20	0.20
5) Frequency and time weighting at 1 kHz	0.20	0.20
6) Long-Term Stability	0.10	0.10
7) Level Linearity on the reference level range	0.30	0.30
8) Tone burst response	0.20	0.30
9) Peak C sound level	0.20	0.35
10) Overload indication	0.20	0.25
11) High-Level Stability	0.10	0.10

Remarks:

1. Indication at the calibration check frequency can not measured because customer does not provide a sound calibrator.
2. The acceptance limit is for the deviated value.
3. Acceptance limits was IEC61672-3:2013 Class 2.
4. The coverage factor $k = 2.00$

-- End of Report --

เอกสารไม่ควบคุม