

เอกสารแนบ 6

เอกสารสอบเทียบเครื่องมือที่ใช้ในการวิเคราะห์

Condition of this calibration result

1. Reference Standard Instruments : This certification is traceable to the international unit of unit maintained through:

Instruments	Model	Serial No.	Certificate No.	Traceable
Documenting Process Calibrator	Fluke 753	43160061	LP24-0014	Measuretronix Limited.
Thermometer with sensor	HI98509	39643D	23T1453	Technology Promotion Association (Thailand-Japan).
Digital Thermo-Hygrometer	HT-771SD	AL07155	24H41	

2. Reference Standard Materials : pH calibration standard traceable thru CPA chem Ltd.

Buffer Solution	Manufacture	Certified Value	Lot Number	Exp. date
pH 4.0	CPA chem	$4.008 \pm 0.006 @ 25^{\circ}\text{C}$	898494	3 June 2024
pH 7.0	CPA chem	$6.985 \pm 0.007 @ 25^{\circ}\text{C}$	898500	28 May 2024
pH 10.0	CPA chem	$10.011 \pm 0.012 @ 25^{\circ}\text{C}$	898502	24 May 2024

Calibration Result :

1. Performing standard curve by Simulator at: -177.5, 0.0, 177.5 mV
(Measurement Electrical Potential) After Adjust Result.

Unit Under Calibration	Nominal Value	Standard Voltage Input	Actual Reading		Uncertainty of Measurement (\pm mV)
			pH	mV	
pH Meter SN 04160019101	4.01	177.5	4.01	177.5	0.097
	7.01	0.0	7.01	0.0	0.058
	10.01	-177.5	10.01	-177.5	0.097

2. Performing three buffer standard curve by using buffer nominal : pH 4,7,10 After Adjustment.

Unit Under Calibration	Standard pH Buffer Solution	Actual Reading (pH)	Actual Reading (mV)	Uncertainty of Measurement (\pm pH)
pH Electrode SN 094430BN	4.008	4.02	159.3	0.010
	6.985	6.99	-13.6	0.011
	10.011	10.04	-187.9	0.014

The report uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

** End of certificate **

Certificate No. : HIT-2410-0320

Page : 1 of 2

CERTIFICATE OF CALIBRATION

Equipment :	pH/mV and EC/TDS/Salinity/Resistivity Meter
Meter Model :	HI5521-02
Probe Model :	HI1131B
Resolution (pH) :	0.01
Manufacturer :	Hanna Instruments
Condition As-Received :	Used Product
Ambient Temperature :	(25 ± 2) $^{\circ}\text{C}$
Customer name :	Okla Testing & Consulting Service Co., Ltd.
	67/35-36, 3RD Floor, Phetkasem 7/1 Road, Wat Tha Pra,
	Bangkok Yai, Bangkok 10600 Thailand
Received date :	28 February 2024
Calibrate date :	4 March 2024
Issue date :	5 March 2024
Calibrated Location :	Hanna Instruments (Thailand) Ltd.
Calibration Procedure :	This calibrator was conducted by using in-house: calibration procedure CP-01, CP-02 by using certified reference material (CRM)

Calibrated by : [REDACTED]

Approved by : [REDACTED]

Authorized Signatory

HANNA
Instruments
(Thailand) Limited

This certificate was certified only for the instrument we calibrated.

This result of calibration was found accurate on date and place of calibration only.

** This certificate may not be reproduced other than in full, except with the prior written **
approval of the head of Hanna Instrument (Thailand)

Result of Calibration: ☒ Without Adjustment ☐ With Adjustment

Calibration Range: 20 °C to 30 °C

Function:

Table 1: This equipment was connected with temperature sensor Model: HI7662-W, S/N: 0615024N.
Dimension: Diameter 3 mm., Length 116 mm.

Immersion Depth (mm)	Standard Reading (°C)	UUC Reading (°C)	Error (°C)	Uncertainty (°C)
110	20.040	20.1	0.1	0.099
110	25.037	25.1	0.1	0.099
110	30.034	30.1	0.1	0.099

UUC*: Unit Under Calibration

End of Certificate of Calibration



CERTIFICATE OF CALIBRATION

Certificate No. : CDT-181-67

Page 1 of 2 Pages

MEASUREMENT ITEM
MANUFACTURER
MODEL/TYPE
SERIAL NUMBER
ID NUMBER
CONDITION AS-RECEIVED
CUSTOMER

: Digital Thermometer with Temperature Sensor
: HANNA INSTRUMENTS
: HI5521
: 04160019101
: -
: Used item
: OKLA Testing and Consulting Service Co., Ltd.
67/35-36 Floor 3, Soi Petchkasem 7/1,
Petchkasem Rd, Watthapra, Bangkokkay, Bangkok 10600.

RECEIVED DATE
MEASUREMENT DATE
ISSUE DATE

: 04 Nov 2024
: 07 Nov 2024
: 11 Nov 2024

ENVIRONMENTAL CONDITIONS:

Ambient condition in the laboratory are as follow:
Temperature : 23.0 ± 3.0 °C
Relative Humidity : 55.0 ± 15.0 %RH

NOTED: The certificate is valid only to the item calibrated on date and place of calibration.

TABULATION OF RESULTS:

The table on next page give the measured values.

Calibration procedure:
The temperature calibration was done by
In-House calibration method as WI-CL-001
according to comparison method with standard
digital temperature indicator and standard
temperature probe. The temperature scale use
was based on ITS-90.

Traceability:

The measurement results are traceable to the
international system of units (SI) through
National Institute of Metrology Thailand (NIMT)
Certificate number: TT-0047-24, Certificate
number: ER-013-24

Reference Used During Calibration:

1. Standard Temperature Probe
Model: STS-100 AS00, Serial No.: 667682 09,
Due date: 26 Mar 2025
2. Digital Temperature Indicator
Model: DTI-1000-A MK II, Serial No.: 671407-
00591 Due date: 21 Oct 2025

Uncertainty of Measurement:

The reported uncertainty of measurement is
based on the standard uncertainty multiplied by
a coverage factor k=2, Which for a normal
distribution corresponds to a coverage
probability of approximately 95%. The standard
uncertainty has been determined in accordance
with the GUM "Evaluation of measurement data
- Guide to the expression of uncertainty in
measurement"

Calibrated by:

Approved signatory:

Calibration Department Manager

Calibration Results

Certificate No. : WK2402-300-865
 Calibration Result of the Accuracy
 Function : Dissolved Oxygen Measurement at 25 °C
 Resolution : 0.01 mg/L

STD Solution	UUC Reading		Error	Uncertainty (± mg/L)
	Before Adjustment	After Adjustment		
0.00	0.32	0.00	0.00	0.15
8.40	9.15	8.37	-0.03	0.33
8.70	9.01	8.65	-0.05	0.33
9.00	9.24	8.92	-0.08	0.33

Unit : mg/L

() Without Adjustment (X) After Adjustment

This certificate may not be reproduced except in full unless permission for the reproduction has been obtained in writing from the laboratory.

**** End of Certificate****

Certificate of Calibration

Certificate No.: WK2402-300-865 Page 1 of 2

Customer : OKLA TESTING & CONSULTING SERVICE CO., LTD.
 67/35-36, 3rd Floor, Petchkasem 7/1, Petchkasem Rd.,
 Watthapra, Bangkok Yai, Bangkok 10600 Thailand.

Instrument : Dissolved Oxygen
 Manufacturer : HANNA
 Model : HI5421
 Serial No. : 04240005101
 Identity No. : KC1A11T8H
 Range : See to data
 Resolution : See to data
 Calibration Method : CP-WK-C03

Ambient Temperature : (25.0 ± 2) °C
 Humidity : (50.0 ± 15) %RH
 Received Date : 27-Feb-24
 Calibrated Date : 27-Feb-24
 Issued Date : 27-Feb-24
 Calibrated Location : In Lab

Reference standard instruments :

Instrument	Serial No.	Certificate No.	Due Date	Traceability to
Zero Oxygen Solution	HI7040L	S0115/20	30-Aug-25	NIST
DO Meter	874477	WK2305-300-241	25-May-24	WK Electric Co.,Ltd.
Digital Thermometer	WK-CT-025	WK2402-300-25	25-Feb-25	WK Electric Co.,Ltd.

NIST : National Institute of Standard and Technology.
 This result calibrate was found accurate as shown on date place of calibrate only
 This certificate is traceability to th International System of Unit (SI)

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence approximately 95 %

Calibrated by : [REDACTED] Approved by : [REDACTED]

Authorized Signatory

This certificate may not be reproduced except in full unless permission for the reproduction has been obtained in writing from the laboratory.

Certificate No. : MT24-5501

Page : 2 of 2

Result : Without adjustment


Resolution : 0.1 °C

Function : Temperature measurement

Calibration point : 104, 140, 160, 180 °C

Calibration point (°C)	Temperature of UUC* at each position (°C)									Uncertainty of measurement (+/- °C)
	Ch.1	Ch.2	Ch.3	Ch.4	Ch.5	Ch.6	Ch.7	Ch.8	Ch.9	
104	104.456	104.237	105.035	104.871	104.694	105.043	104.255	104.486	104.956	0.67
140	141.286	140.733	141.403	141.502	140.674	141.611	139.677	141.949	141.131	0.87
160	161.706	160.284	161.505	161.802	160.657	161.912	159.449	161.991	161.106	0.91
180	181.164	179.786	180.990	181.272	180.128	181.374	178.909	181.619	180.617	0.90

Setting temperature (°C)	Indicating Temperature (°C)	Measured stability (+/- °C)	Measured uniformity (°C)	Overall variation (°C)
104.0	104.1 to 104.3	0.53	1.0	1.6
140.0	140.1 to 140.3	0.61	2.1	3.1
160.0	160.1 to 160.3	0.65	2.1	3.6
180.0	180.1 to 180.3	0.64	2.2	3.6

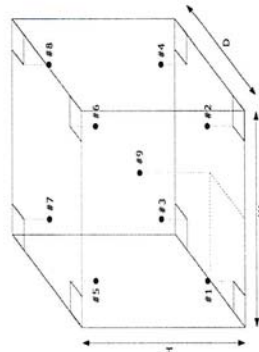

- #1 Lower Left Front
- #2 Lower Right Front
- #3 Lower Left Rear
- #4 Lower Right Rear
- #5 Upper Left Front
- #6 Upper Right Front
- #7 Upper Left Rear
- #8 Upper Right Rear
- #9 Geometric Center

UUC* = Unit under calibration
Uniformity = Maximum and Minimum difference of measured temperature at any probes and the measured temperature at the reference and same time.
Overall Variation = Difference of temperature value between the maximum and minimum any time.
Stability = One half of the maximum difference of measured temperatures at any one probe.

Certificate of Calibration

Certificate No. : MT24-5501

Page : 1 of 2

Customer : บริษัท โกลา เทคโนโลยี แอนด์คอนโซลิ่ง เซอร์วิส จำกัด
Address : 67/35-36 ชั้น 3 ซอยเพชรเกษม 7/1 แขวงวัดท่าพระ เขตบางกอกใหญ่ กรุงเทพมหานคร 10600

Description : Drying Oven
Manufacturer : N/A
Model : SOV70B
Serial No. : KWF2021021902
Identification No. : OKLA-LAB-013/170621
Calibration Place : Laboratory

Order No. : 2026/24
Received date : Jun 24, 2024
Calibration date : Jun 24, 2024
Environment Condition :
Temperature : (25±10) °C
Humidity : (50±30) %RH

Calibration Method : Calibration were conducted using In-house calibration procedure CP-MT-006 According to comparison with LXI Data Acquisition Switch Unit with sensor. The calibration methods based on Euramet Calibration Guide No.20 - guidelines on the Calibration of Temperature and/or Humidity Controlled Enclosures.

Reference Standard Instruments :

Instrument	Model	Serial No.	Certificate No.	Due Date
LXI Data Acquisition Switch Unit with Sensor	34972A	MY57003222	MT23-5938	Oct 05, 2024

The effect that the result relate only to the items calibrated. It was found accurate as shown on date and place of calibration only.

Traceability : This measurement are traceable to the International System of Unit (SI), through National Institute of Metrology Thailand (NIMT)

The reported expanded uncertainty of measurement was based on standard uncertainty multiplied by coverage factor $k = 2$, providing a level of confidence of not less than 95%



Calibrated by :
Approved by :
Issue date : Jun 28, 2024

This calibration certificate shall not be reproduced other than in full except with the prior written approval of Inctech Metrological Center Co.,Ltd

Certificate of Calibration

Certificate No. : 67-400117-1


Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Function : Temperature measurement

This instrument was setting air ventilation at position 0 (close)

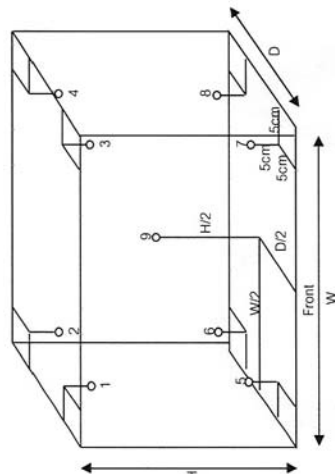

Test Point (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Temperature (°C) @ Sensor No.									Uncertainty (± °C)
			1	2	3	4	5	6	7	8	9	
20.0	20.0	20.0	20.46	20.25	19.60	19.58	19.84	19.64	19.45	19.59	20.01	0.34

Test Point (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Uniformity (°C)	Measured Stability (°C)	Overall Variation (°C)
20.0	20.0	20.0	0.589	0.073	1.129

Remark The uncertainty is not combine uniformity of the air chamber

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k=2$, providing a level of confidence of approximately 95%

-oOo-



Approved by :

Laboratory Manager

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.

Certificate of Calibration

Certificate No. : 67-400117-1

Page : 1 of 2

Submitted by : Okla Testing & Consulting Service Co., Ltd.

67/35-36, 3rd Floor, Petchkasem 7/1, Petchkasem Rd.,

Wathapra, Bangkok Yai, Bangkok 10600 Thailand

Equipment : Temperature controlled enclosure (Incubator)

Manufacturer : S-Cool

Model : SM 61 M

Range : N/A °C

Resolution : 0.1 °C

Serial No. : 18021147

ID No. : OKLA-LAB-011/190

Environment : On site calibration was carried out at the Laboratory.

Okla Testing & Consulting Service Co., Ltd.

Ambient Temperature : (32.0 to 33.0) °C

Relative Humidity : (50 to 55) %

Line Voltage : (221.0 to 223.0) V

Date of Received : 26 February 2024

Date of Calibration : 26 February 2024

Date of Issue : 29 February 2024

Calibrated by : Kittisak Kokaeo

Calibration Method : CAL-M4004, TLAS G-20

The temperature scale used was based on ITS-90

Reference Standard Instruments : This certification is traceable to the International System of Units

Standard Digital Thermometer with RTD Probe

ID No. 400046 & 400047

Cert. No. 67-400047-2

Due Date 26 Jul 2024

Traceability National Institute of Metrology Thailand (NIMT)



Approved by :

Laboratory Manager

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.

Certificate No. : J048-TC24021201

Page : 2 of 3

Calibration Report

Equipment : Refrigerator
Model : SPB-0500
Environment : Ambient Temperature (24.3 to 24.9) °C
Relative Humidity (45.3 to 51.9) %
Line Voltage (226 to 228) V_{ac}
Manufacturer : SANDEN
Serial No : SPB0500-231007454

Detail of this calibration result.:

1. This instrument was calibrated by insert 9 standards Resistance Thermometer Detector, in to the chamber, under no load condition in according to TLAS G-20-1/02-08 (E).
2. The temperature scale used was based on ITS-90.
3. Reference standards instrument :

Instrument	Model	Serial No./ID No.	Certificate No.	Due Date
Data Acquisition Switch unit	34972A	MY49010832	QR23-2679	15 November 2024
Resistance Thermometer Detector	100 ohm	RTD505(01 to 10)	QR23-2679	15 November 2024

4. This certificate was certified only for the instrument we calibrated.
5. The measured values in this report refer to the time of examination.
6. This certificate is traceable to SI Unit through Quality Reborn Co.,Ltd.
NSC - ONSC accredited no. Calibration 0292

7. Condition of calibrated item : Good

UUC Description :

Operation time 5 Hour 00 Minute Calibration point 2.0, 4.0, 6.0 °C

The air ventilation of the instrument was set at position.

Fresh Air Damper

<input type="checkbox"/>	Open	<input type="checkbox"/>	Position	<input type="checkbox"/>	Min	<input type="checkbox"/>	Medium	<input type="checkbox"/>	Max
<input type="checkbox"/>	Close								
<input checked="" type="checkbox"/>	X								

8 Result of calibration :

(X) Without adjustment () After adjustment

Certificate No. : J048-TC24021201

Page : 1 of 3

Certificate of Calibration

Customer : Okla Testing & Consulting Service Co., Ltd.
Address : 67/35-36, 3rd Floor, Phetkasem 7/1 Rd.,
Wathapra, Bangkokkayai, BKK. 10600

Equipment : Refrigerator
Manufacturer : SANDEN
Model : SPB-0500
Serial No. : SPB0500-231007454
ID No. : -
Resolution : 0.1 °C
Location of Calibration : Central Laboratory FL.3
Reference Job No. : JB24048
Received Request Date : 12 February 2024
Calibrated by : Pawut Wongnarakornkul
Date of Calibration : 12 February 2024

Approved by :



Date of Issue : 13 February 2024

The uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval the Megafil Co.,Ltd.



Certificate of Calibration

Certificate No. : 67-400117-4

Page : 1 of 2

Submitted by :

Okla Testing & Consulting Service Co., Ltd.

67/35-36, 3rd Floor, Petchkasem 7/1, Petchkasem Rd.,

Watthapra, Bangkok Yai, Bangkok 10600 Thailand

Equipment :

Water Bath

Manufacturer : LabTech

Model : LWB-222A

Range : N/A °C

Resolution : 0.01 °C

Serial No. : BCCLJ23001C

ID No. : OKLA-LAB-008/122011

Environment :

On site calibration was carried out at the Laboratory,

Okla Testing & Consulting Service Co., Ltd.

Ambient Temperature : (32.0 to 33.0) °C

Relative Humidity : (50 to 55) %

Line Voltage : (221.0 to 223.0) V

Date of Received : 26 February 2024

Date of Calibration : 26 February 2024

Date of Issue : 29 February 2024

Calibrated by : Permpoon Chanpu

Calibration Method :

This instrument was calibrated by In-house method CAL-M4006 based on ASTM E715-80

The temperature scale used was based on ITS-90

Reference Standard Instruments : This certification is traceable to the International System of Units

Standard Digital Thermometer with RTD probe

ID No. Cert. No.

Traceability

400029 & 400043

National

Due Date

25 Apr 2024

Thailand (NIMT)

Approved by :

(Signature)

Laboratory Manager

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co., Ltd.




Certificate No. : J048-TC24021201

Page : 3 of 3

Result of Calibration

Sensor installation at nine locations as show in figure.

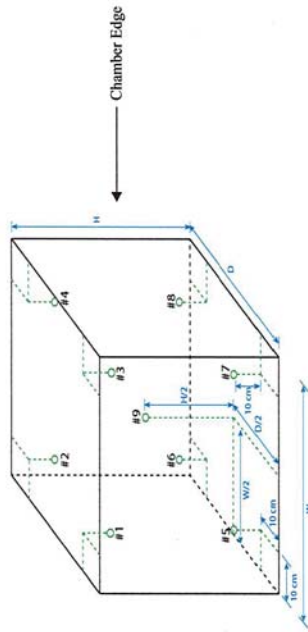Chamber capacity (W x H x D) : (0.55 x 1.61 x 0.42) m : 0.37 m³

Position	1	2	3	4	5	6	7	8	9
Ref. Std/ID No.:	RTD50500	RTD50502	RTD50503	RTD50504	RTD50505	RTD50506	RTD50507	RTD50508	RTD50509

Temperature distribution

Cal. Point (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Temperature (°C) @ Sensor No. (Sensor No.9 is REF)									Uncertainty (± °C)
			1. °C									
			1	2	3	4	5	6	7	8	9	
2.0	2.0	2.0	2.03	1.26	1.94	1.31	3.06	2.95	2.21	2.15	2.17	0.44
4.0	4.0	4.0	3.96	3.22	3.84	3.31	5.05	4.91	4.19	4.18	4.14	0.44
6.0	6.0	6.0	5.85	5.16	5.88	5.32	7.07	6.91	6.18	6.24	6.10	0.44

Chamber performance

Cal. Point (°C)	Setting Temperature (°C)	Indicating Temperature (°C)		Measured Uniformity (°C)	Measured Stability (± °C)	Overall Variation (°C)
		Min	Average			
2.0	2.0	2.0	2.0	1.07	0.19	2.06
4.0	4.0	4.0	4.0	1.09	0.22	2.04
6.0	6.0	6.0	6.0	0.98	0.24	2.18

Note: The quoted uncertainty include Stability and 20% of Uniformity.

Stability = One-half of the greatest maximum difference of measured temperatures at any one sensor.

Uniformity = The maximum difference of measured temperatures at any sensors and measured temperature at the reference location which are observed at the same time.

Overall Variation = The Difference of the maximum and minimum measured temperatures throughout observation.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k = 2.00, providing a level of confidence of approximately 95%.

- End of Certificate -

Megafil Co., Ltd.

MG-FM-7.8-002, R00 (01/07/19)



Certificate of Calibration

Certificate No. : 67-200069-1

Page : 1 of 2

Submitted by :

Okla Testing&Consulting Service Co.,Ltd.

67/35-36, 3rd Floor, Petchkasem 7/1, Petchkasem Rd.,

Wathapra, Bangkok Yai, Bangkok 10600 Thailand

Equipment :

Electronic Balance

Manufacturer : Sartorius

Model : BSA224S-CW

Serial No. : 35790699

Capacity : 200 g Resolution : 0.0001 g

On site calibration was carried out at t/Laboratory Environmental,Okla

Testing&Consulting Service Co.,Ltd.

Ambient Temperature : (28.4 to 28.5) °C

Relative Humidity : (49.4 to 51.1) %

Air Pressure : 1012.0 mbar

Date of Received :

26 February 2024

Date of Calibration :

26 February 2024

Date of Issue :

27 February 2024

Calibrated by :

Akaradath Thippichai

Calibration Method :

In-house method CAL-M2001 based on UKAS Publication ref : LAB 14

Edition 7 - November 2022

Reference Standard Instruments : This certification is traceable to the International System of Units

Standard Weights

ID No.

Traceability

E261-E264

Cert. No.

C02232088

Due Date

08 Nov 2024 National Institute of Metrology (Thailand), (NIMT)

Approved by :

Laboratory Manager

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.

Certificate of Calibration


Certificate No. : 67-400117-4

Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Function : Temperature measurement

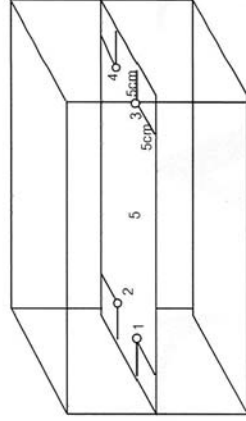

Front

Test Point (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Temperature (°C) @ Sensor					Uncertainty (± °C)	Measured Uniformity (°C)	Measured Stability (°C)	
			No.	1	2	3	4				5
60	As Mark 60	-		60.02	59.97	60.02	59.95	60.05	0.53	0.69	0.40

$$\sqrt{0.53^2 + 0.69^2} = 0.881$$

Remark The uncertainty is not combine uniformity of the water bath

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

-o0o-

CERTIFICATE OF CALIBRATION

Certificate No. : CDT-116-67

Page 1 of 2 Pages

MEASUREMENT ITEM
MANUFACTURER
MODEL/TYPE
SERIAL NUMBER
ID NUMBER
CONDITION AS-RECEIVED
CUSTOMER

: Digital Thermometer with Temperature Sensor

: EUTECH

: ECO SCAN TEMPS

: 816366

: -

: Used item

: OKLA Testing and Consulting Service Co., Ltd.

: 67/35-36 Floor 3, Soi Petchakaset 7/1,

: Petchakaset Rd, Watthapra, Bangkokkayk, Bangkok 10600.

RECEIVED DATE

MEASUREMENT DATE

ISSUE DATE

: 01 Jul 2024

: 03 Jul 2024

: 04 Jul 2024

ENVIRONMENTAL CONDITIONS:

Ambient condition in the laboratory are as follow:

Temperature : 23.0 ± 3.0 °C

Relative Humidity : 55.0 ± 15.0 %RH

NOTED: The certificate is valid only to the item calibrated on date and place of calibration.

TABULATION OF RESULTS:

The table on next page give the measured values.

Calibration procedure:

The temperature calibration was done by In-House calibration method as WI-CI-001 according to comparison method with standard digital temperature indicator and standard temperature probe. The temperature scale use was based on ITS-90.

Traceability:

The measurement results are traceable to the international system of units (SI) through National Institute of Metrology Thailand (NIMT) Certificate number: TT-0047-24, Certificate number: ER-0101-23

Reference Used During Calibration:

1. Standard Temperature Probe
Model: STS-100 A500, Serial No.: 667682-09,
Due date: 26 Mar 2025
2. Digital Temperature Indicator
Model: DTI-1000-A MKII, Serial No.: 671407-00591 Due date: 14 Sep 2024

Uncertainty of Measurement:

The reported uncertainty of measurement is based on the standard uncertainty multiplied by a coverage factor $k=2$, Which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty has been determined in accordance with the GUM 'Evaluation of measurement data - Guide to the expression of uncertainty in measurement'

Calibrated by:

Approved signatory:

Calibration Department Manager

Certificate of Calibration

Certificate No. : 67-200069-1

Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Departure of indication from nominal value

Nominal Value (g)	Correction (g)	Uncertainty \pm (g)
0.01	0.0000	0.00011
0.05	0.0000	0.00011
0.1	0.0000	0.00011
0.2	0.0000	0.00011
0.5	0.0000	0.00011
1	0.0000	0.00011
10	0.0000	0.00011
50	0.0000	0.00014
100	0.0000	0.00020
150	0.0001	0.00038
200	0.0002	0.00038

This result of calibration was found accurate as shown on date and place of calibration only.


This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2.00$, providing a level of confidence of approximately 95%

Eccentric error

Load test : 50 g

A	B	C	D	E
-0.0001	0.0001	0.0001	0.0000	0.0000

g



Repeatability

Load test : 200 g

Sidev. : 0.00000 g

-o0o-

CERTIFICATE OF CALIBRATION

Certificate No. : CRT-061-67

Page 1 of 2 Pages

MEASUREMENT ITEM
MANUFACTURER
MODEL/TYPE
SERIAL NUMBER
ID NUMBER
CONDITION AS-RECEIVED
CUSTOMER

: Digital Thermo Hygrometer
: KEPLER Instrument
: KTH-02
: 234011889
: -
: Used Item
: Olda Testing and consulting services Co., Ltd.
67/35-36, 3rd Fl, Petchkasem soi 7/1, Wat Thapra,
Bangkokkylai, Bangkok, Thailand 10600.

RECEIVED DATE
MEASUREMENT DATE
ISSUE DATE

: 16 Dec 2024
: 19 Dec 2024
: 19 Dec 2024

ENVIRONMENTAL CONDITIONS:

Ambient condition in the laboratory are as follow:
Temperature : 23.0 ± 3.0 °C
Relative Humidity : 55.0 ± 15.0 %RH

NOTED: The certificate is valid only to the item calibrated on date and place of calibration.

TABULATION OF RESULTS:

The table on next page give the measured values.

Calibrated by: [REDACTED]

Approved signatory: [REDACTED]

Calibration Department Manager



Result of Calibration: ☒ Without Adjustment ☐ With Adjustment

Calibration Range: 20 °C to 30 °C

Function:

Table 3: This equipment was connected with Thermocouple sensor type K.
Dimension: Diameter 3 mm. Length 116 mm.

Immersion Depth (mm)	Standard Reading (°C)	UUC Reading (°C)	Error (°C)	Uncertainty (°C)
110	20.047	20.1	0.0	0.26
110	25.043	25.0	0.0	0.26
110	30.034	30.0	0.0	0.26

UUC*: Unit Under Calibration

End of Certificate of Calibration



Continuation of Certificate of Calibration Number: CRT-061-67

Measurement Results:

The results of calibration and associated measurement uncertainties are reported in the table below.

Result of Calibration: ☒ Without Adjustment ☐ With Adjustment

Table 1: The results of calibration of air temperature are reported in table below.

Calibration Range: 20 °C to 30 °C

Determined (°C)	Standard Reading (°C)	UUC Reading (°C)	Error (°C)	Uncertainty ±(°C)
20.00	20.06	20.6	0.5	0.31
25.00	25.04	25.3	0.3	0.31
30.00	30.04	29.6	-0.4	0.31

Table 2: The results of calibration of relative humidity at 23 °C are reported in table below.
Calibration Range: 35%RH to 70%RH

Air Temperature (°C)	Standard Reading (%RH)	UUC Reading (%RH)	Error (%RH)	Uncertainty ±(%RH)
23.04	34.74	36	1	1.0
23.04	44.71	43	-2	1.3
23.00	59.68	58	-2	1.8
23.03	69.61	66	-4	1.8

UUC*: Unit Under Calibration

End of Certificate of Calibration

