

ภาคผนวกที่ 5
เอกสารสอบเทียบเครื่องมือตรวจวัด

ภาคผนวกที่ 5-1
เอกสารสอบเทียบเครื่องมือตรวจวัดคุณภาพอากาศ

CERTIFICATE OF CALIBRATION

Certificate No. : COF-017-67

Page 1 of 2 Pages

MEASUREMENT ITEM : Top Load Orifice
MANUFACTURER : TISCH
MODEL/TYPE : TE-5025A
SERIAL NUMBER : 710725
ID NUMBER : -
CONDITION AS-RECEIVED : Used item
CUSTOMER : Pacific Laboratory Co., Ltd.
14/5358 Moo14, T.Bang Bua Thong, A.Bang Bua Thong,
Nonthaburi 11110, Thailand.

RECEIVED DATE : 28 May 2024
MEASUREMENT DATE : 31 May 2024
ISSUE DATE : 31 May 2024

ENVIRONMENTAL CONDITIONS:

Ambient condition in the laboratory are as follow:

Temperature	: 23.0 ± 3.0	°C
Relative Humidity	: 55.0 ± 15.0	%RH
Atmospheric Pressure	: 1010 ± 10	hPa

CALIBRATION CONDITION:

Preconditioning : 24 hours at ambient conditions.
Measurement Condition : The average values during measurement are 23.1 °C and 50.4 %RH.

NOTED: The certificate is valid only to the item calibrated on date and place of calibration.

TABULATION OF RESULTS:

The table on next page give the measured values.

Calibration procedure:

The Orifice gas flow device was calibrated against Standard Rotary Displacement Meter (Roots Meter) Model G65/IMC/W2-dp. The WI-CL-004 was used as a calibration guideline.

Traceability:

This certificate provides a traceability of the measurement to recognized the national standards, and to realization of the international system of units (SI) through the NIMT (National Metrology Institute of Thailand) via Certificate number: MW-0063-23.

Uncertainty of Measurement:

The reported uncertainty of measurement is based on the standard uncertainty multiplied by a coverage factor $k=2$, Which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty has been determined in accordance with the GUM 'Evaluation of measurement data - Guide to the expression of uncertainty in measurement'

Calibrated by:

- ☒ Mr. Sorawit Thachalad
☐ Miss Jitraporn Lertsomphol



Approved signatory:

Calibration Department Manager

MEASUREMENT RESULTS:

The Orifice gas flow device was calibrated by direct comparison method with the Standard Rotary Displacement Meter (Roots Meter). The Humid air was used as a medium in the system. The standard conditions are 25°C (298.15 K) and 760 mmHg for standard temperature and standard pressure respectively.

Table 1: The results of Q Standard calibration data

Plate	Flow rate m^3/min	Pressure [Pa] mmHg	Temperature [Ta] °C	Temperature [Tm] °C	Δp_{meter} mmHg	$\Delta p_{Orifice}$ inH ₂ O	y	Standard Flow [Q_s] m^3/min
1	0.702	752.536	23.17	22.37	49.860	1.691	1.298	0.655
2	1.002	752.502	23.34	22.68	63.856	3.329	1.821	0.915
3	1.110	752.584	23.41	22.80	42.943	4.353	2.082	1.044
4	1.167	752.462	23.62	22.97	32.314	4.956	2.220	1.113
5	1.423	752.441	23.74	23.07	29.684	7.471	2.725	1.362

Slope (m): 2.01598
 Intercept (b): -0.02301
 Correlation coefficient (r): 0.99985
 Uncertainty ($k=2$): 0.015 m^3/min

Table 2: The results of Q actual calibration data

Plate	Flow rate m^3/min	Pressure [Pa] mmHg	Temperature [Ta] °C	Temperature [Tm] °C	Δp_{meter} mmHg	$\Delta p_{Orifice}$ inH ₂ O	y	Standard Flow [Q_a] m^3/min
1	0.702	752.536	23.17	22.37	49.860	1.691	0.816	0.657
2	1.002	752.502	23.34	22.68	63.856	3.329	1.145	0.919
3	1.110	752.584	23.41	22.80	42.943	4.353	1.310	1.049
4	1.167	752.462	23.62	22.97	32.314	4.956	1.398	1.119
5	1.423	752.441	23.74	23.07	29.684	7.471	1.717	1.370

Slope (m): 1.26266
 Intercept (b): -0.01445
 Correlation coefficient (r): 0.99985
 Uncertainty ($k = 2$): 0.015 m^3/min

End of Certificate of Calibration



CALIBRATION TEST REPORT FOR Partisol Air Sampler

Calibrated Date: 27 January 2025
Calibrated Due on: 26 January 2026

Report No: PM-202501027

Instruments Information

Description : Thermo Scientific Partisol 2025i
Sequential Air Sampler

Model : 2025i

Sample flow control and reporting : 5 - 18 LPM

Serial No. : 2025i2 0587 1403

Instrument used for calibration [STD]

Description : Flow Meter

BIOS DryCal DC-Lite

Model : DCL-M REV. 1.08


Range : 200 ml/min - 20 L/min


Serial No. : 5016

Environment : Temperature 25.5 °C Humidity: 51 %RH

Calibration Report

Filter	Set Flow Instrument (L/Min)	Current Flow Instrument reading (L/Min)	Actual Flow Reference standard (L/Min)	Error	Drift%
47 mm	15.00	15.00	14.93	-0.07	0.49
	16.67	16.67	16.61	-0.06	0.36
	18.34	18.34	18.12	-0.22	1.20

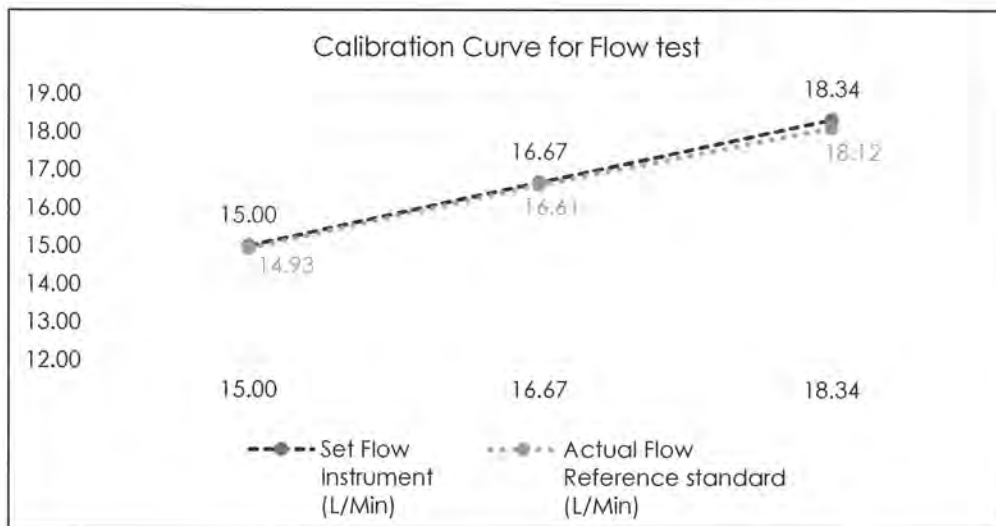

Calibrate By : 

MR. KITTISAK JANTANA

Approve by : 

MR.

CALIBRATION TEST REPORT FOR Partisol Air Sampler

Calibrated Date: 27 January 2025
Calibrated Due on: 26 January 2026

Report No: PM-202501029

Instruments Information

Description : Thermo Scientific Partisol 2025i
Sequential Air Sampler

Model : 2025i

Sample flow control and reporting : 5 - 18 LPM

Serial No. : 2025i2 0585 1402

Instrument used for calibration [STD]

Description : Flow Meter

BIOS DryCal DC-Lite

Model : DCL-M REV. 1.08


Range : 200 ml/min - 20 L/min


Serial No. : 5016

Environment : Temperature 25.5 °C Humidity: 51 %RH

Calibration Report

Filter	Set Flow Instrument (L/Min)	Current Flow Instrument reading (L/Min)	Actual Flow Reference standard (L/Min)	Error	Drift%
47 mm	15.00	15.00	14.91	-0.09	0.62
	16.67	16.67	16.58	-0.09	0.54
	18.34	18.34	18.21	-0.13	0.70

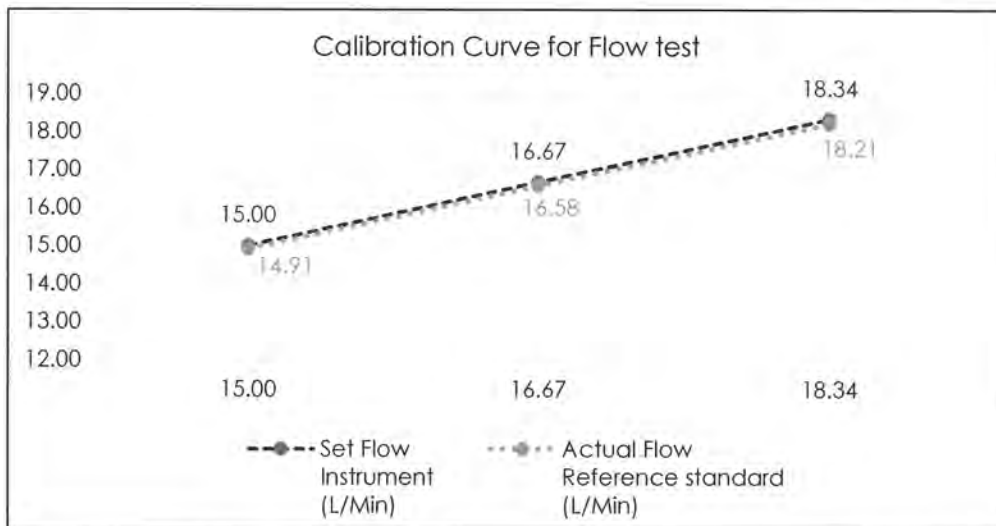

Calibrate By : 
MR. KITTISAK JAN

Approve by : ()

MR.

CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhprachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech_cal@yahoo.com, calibratech_cal@hotmail.com



NSC-TISI-TIS 17025
CALIBRATION 0030

Certificate of Calibration

Certificate No. : 67-200273-1

Page : 1 of 2

Submitted by : Pacific Laboratory Co., Ltd.

14/5358 Moo 14, T.Bang Bua Thong, A.Bang Bua Thong, Nonthaburi 11110 Thailand

Equipment : Electronic Balance

Manufacturer : SHIMADZU

Model : AP225WD

Serial No. : D316301828

ID No. : LAB-BL-003

Capacity : 220000 mg

Resolution : 0.01mg/102000mg, 0.1mg/220000mg

Environment : On site calibration was carried out at the Laboratory, Pacific Laboratory Co., Ltd.

Ambient Temperature : (26.2 to 26.4) °C

Relative Humidity : (34.0 to 35.4) %

Air Pressure : 1007.0 mbar

Date of Received : 30 July 2024

Date of Calibration : 30 July 2024

Date of Issue : 31 July 2024

Calibrated by : Akaradath Thippichai

Calibration Method : In-house method CAL-M2001 based on UKAS Publication ref : LAB 14

Edition 7 - November 2022

Reference Standard Instruments : This certification is traceable to the International System of Units

Standard Weights

ID No.	Cert. No.	Due Date	Traceability
E261-E2624	C02232088	08 Nov 2024	National Institute of Metrology (Thailand), (NIMT)

Approved by :

(Surach

Laboratory Manager

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



CAL-F0031-03

CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhprachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech.cal@yahoo.com, calibratech.cal@hotmail.com

Certificate of Calibration

Certificate No. : 67-200273-1

Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Departure of indication from nominal value

Nominal Value (mg)	Correction (mg)	Uncertainty \pm (mg)
1	0.01	0.012
10	0.01	0.012
50	0.01	0.012
100	0.01	0.014
1000	0.00	0.026
2000	0.01	0.034
5000	0.00	0.043
20000	0.00	0.071
50000	0.01	0.11
100000	0.00	0.20
150000	0.0	0.38
200000	0.0	0.38


This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2.06$, providing a level of confidence of approximately 95%

Eccentric error

Load test : 50000 mg

A	B	C	D	E	
0.00	0.00	0.01	0.00	0.00	mg



Repeatability

Load test : 200000 mg

Stdev. : 0.053 mg

- oOo -





บริษัท เอ็นไวร์ เซอร์วิส จำกัด

42 รามอินทรา 14 แยก 9 แขวงจันทบุรี เขตบางเขน กรุงเทพฯ 10230 โทรศัพท์ 02-9435814-5 โทรสาร 02-9438201
บริษัท เอ็นไวร์ เซอร์วิส จำกัด
ENVIR SERVICE CO., LTD. 42 Raminthra 14 yeak 9, Tha Rang, Bangkok, Bangkok 10230 Tel : 02-9435814-5 Fax : 02-9438201

Analyzer Performance Test

Calibrated Date: 7 August 2024

Instruments Information

Analyzer Type: SO2 Analyzer Model: 43C	Manufacturer Thermo Environmental S/N: 0601114-787
---	---

Calibration System


Calibrator Unit	Standard Gas
Dilutor Model Dasibi Model 5008 S/N: 705 ZERO AIR Generator API MODEL 701 S/N: 1924	NO Conc 46.05 PPM SO2 Conc 46.01 PPM CO Conc 4.487 PPM Expire Date: 19 Sep. 2020

Environment: Temperature 25.5 °C

Humidity: 51 %RH

Calibration Report

Status	Zero			Span		
	Reference (PPB)	Reading (PPB)	Drift (PPB)	Reference (PPB)	Reading (PPB)	Drift%
Before	0.0	0.1	0.1	400.0	394.9	-1.3
After	0.0	0.0	0.0	400.0	400.0	0.0

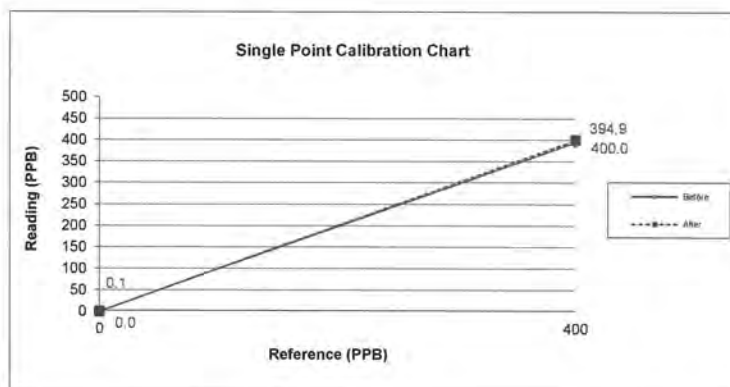

Calibrate By :

Mr.PASAG



บริษัท เอ็นไวร์ เซอร์วิส จำกัด

42 รามอินทรา 14 แยก 9 แขวงท่าแร้ง เขตบางเขน กรุงเทพฯ 10230 โทรศัพท์ 02-9435814-5 โทรสาร 02-9438201
บริษัท เอ็นไวร์ เซอร์วิส จำกัด
ENVIR SERVICE CO., LTD. 42 Raminthra 14 yeak 9, Tha Rang, Bangkhen, Bangkok 10230 Tel : 02-9435814-5 Fax : 02-9438201

Analyzer Performance Test

Calibrated Date: 9 August 2024

Instruments Information

Analyzer Type: NO/NO ₂ /NO _x Analyzer Model: 42C	Manufacturer: Thermo Environmental S/N: 65850-350
---	--

Calibration System

Calibrator Unit	Standard Gas
Dilutor Model Dasibi Model 5008 S/N: 705 ZERO AIR Generator API Model 701 S/N: 1924	NO Conc 46.05 PPM SO ₂ Conc 46.01 PPM CO Conc 4,487 PPM Expire Date: 19 Sep. 2020

Environment: Temperature 25.5 °C


Humidity: 51 %RH

Calibration Check (Before adjust)

GAS	Zero			Span		
	Reading Value (ppb)	Expected Value (ppb)	Drift (ppb)	Reading Value (ppb)	Expected Value (ppb)	Drift%
NO	0.1	0.0	0.1	397.2	400.0	-0.7
NO _x	0.1	0.0	0.1	400.0	400.0	0.0

Calibration Check (After adjust)

GAS	Zero			Span		
	Reading Value (ppb)	Expected Value (ppb)	Drift (ppb)	Reading Value (ppb)	Expected Value (ppb)	Drift%
NO	0.0	0.0	0.0	400.0	400.0	0.0
NO _x	0.0	0.0	0.0	400.0	400.0	0.0

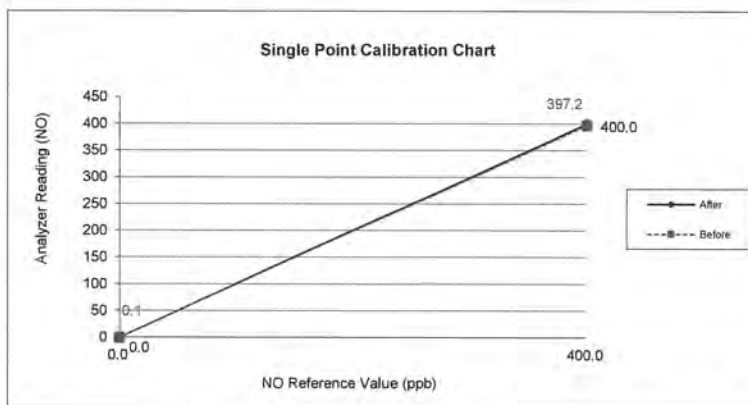

Calibrate By : Mr. Pasagor



บริษัท เอ็นไวร์ เซอร์วิส จำกัด

42 รามอินทรา 14 แยก 9 แขวงท่าแร้ง เขตบางเขน กรุงเทพฯ 10230 โทรศัพท์ 02-9435814-5 โทรสาร 02-9438201
บริษัท เอ็นไวร์ เซอร์วิส จำกัด 42 Ramintra 14 yeak 9, Tha Rang, Bangkhen, Bangkok 10230 Tel : 02-9435814-5 Fax : 02-9438201
ENVIR SERVICE CO., LTD.

Analyzer Performance Test

Calibrated Date: 11 August 2024

Instruments Information

Analyzer Type: CO Analyzer Model: 48C	Manufacturer Thermo Environmental S/N: 65774-350
--	---

Calibration System


Calibrator Unit	Standard Gas
Dilutor Model Dasibi Model 5008 S/N: 705 ZERO AIR Generator API MODEL 701 S/N: 1924	NO Conc 46.05 PPM SO2 Conc 46.01 PPM CO Conc 4.487 PPM Expire Date: 19 Sep. 2020

Environment: Temperature 25.5 °C

Humidity: 51 %RH

Calibration Report

Status	Zero			Span		
	Reference (PPM)	Reading (PPM)	Drift (PPM)	Reference (PPM)	Reading (PPM)	Drift%
Before	0.0	0.1	0.1	45.0	44.8	-0.4
After	0.0	0.0	0.0	45.0	45.0	0.0

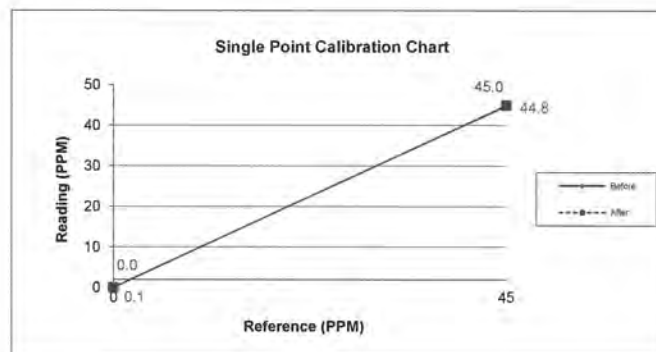

Calibrate By :

Mr. PAS

Analyzer Performance Test

Calibrated Date: 24 April 2024

Instruments Information

Analyzer Type : Methane-NMHC Analyzer

Manufacturer : Thermo Environmental

Model : 55C

Serial Number : 55C-0515611965

Calibrator Unit

Dilutor Model : Dasibi Model 5008

Serial Number : 705

ZERO AIR Generator : API MODEL 701

Serial Number : 1924

Standard Gas Concentration

Methane (CH₄) 183.0 PPM

Propane 59.1 PPM

Cylinder number 4860

Expire Date: 6 Dec. 2025


Environment : Temperature 25.5 °C Humidity: 51 %RH


Calibration Report (Before adjust)

Status	Zero			Span		
	Reference (PPM)	Reading (PPM)	Drift (PPM)	Reference (PPM)	Reading (PPM)	Drift%
Methane	0.0	0.1	0.1	183.0	181.2	-1.0
NMHC	0.0	0.1	0.1	59.1	58.3	-1.4

Calibration Report (After adjust)

Status	Zero			Span		
	Reference (PPM)	Reading (PPM)	Drift (PPM)	Reference (PPM)	Reading (PPM)	Drift%
Methane	0.0	0.0	0.0	183.0	182.7	-0.2
NMHC	0.0	0.0	0.0	59.1	59.0	-0.2

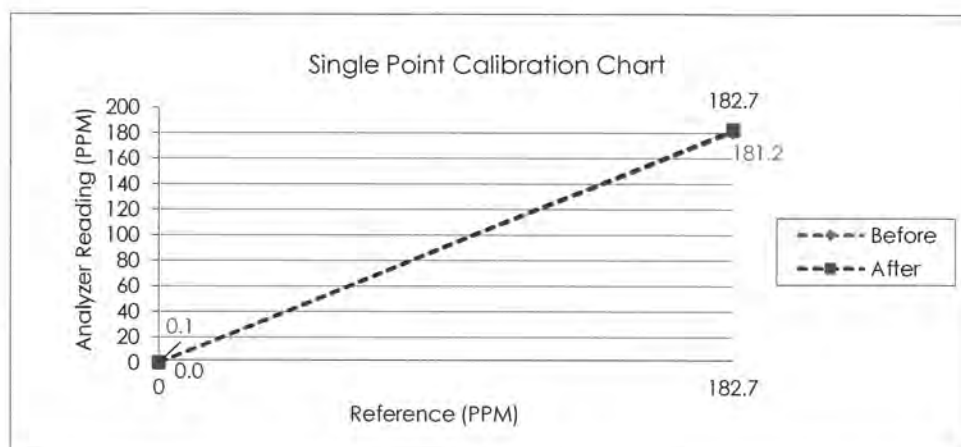

Calibrate By : 

MR. K

Approve by : 

M

ภาคผนวกที่ 5-2
เอกสารสอบเทียบเครื่องมือตรวจวัดระดับเสียง



Professional Calibration & Services Co., Ltd.

50/888, 50/889 Moo 2, Rungsit-Nakornnayok Rd., Bungeeetho, Thunyaburi,
Pathumthani 12130 Thailand
Tel : (+66)2150-6641 (Autoline), (+66)2569-5158
Email : info@p-cal.com www.p-cal.com



Certificate of Calibration

Certificate Number : EL41650/24
Control Number : PCAL153035
Customer Control : -
Description : Sound Calibrator
Manufacturer : SOUNDTEK
Model : ST-120
Serial Number : 211203764
Customer : Pacific Laboratory Co., Ltd.
14/5358 Moo 14, Tambol Bang Bua Thong, Amphoe Bang Bua Thong,
Nonthaburi 11110

Date of Receipt : 22-Aug-24
Date of Calibration : 23-Aug-24
Environment : Temperature $23\text{ }^{\circ}\text{C} \pm 2\text{ }^{\circ}\text{C}$
Relative Humidity $50\text{ \%} \pm 20\text{ \%}$
Calibration Method : Calibration Procedure Number CP-EL35
Calibration Results : See data attached



Page 1 of 3

The reported uncertainty is based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%.

This certificate is issued in accordance with ISO/IEC17025 and the conditions of accreditation granted by the Accreditation Body which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory. The results relate only to the item calibrated.

This certificate shall not be reproduced other than in full except without the prior written approval of the Head of Calibration Laboratory of Professional Calibration & Services Co., Ltd.

Calibrated By

Mr. Nonpawit Wiseschoo

Authorized Signature

(Mr. Ma

27-Aug-24

Issued Date

CALIBRATION REPORT

Professional Calibration & Services Co.,Ltd.

Certificate Number : EL41650/24

Page 2 of 3

Equipment Standards Used

Description	Serial No.	Traceability to	Certificate No.	Cal. Due Date
Sound Level Meter	030606101	ANAB : AC-2590	EL12298/24	27-Mar-25
Sound Calibrator	125626778	NSC : Calibration 0037	EEL.BP. 161/0167	04-Feb-25

Condition as received : Normal

Definitions :-

- * ANAB - The ANSI National Accreditation Board
- * NSC - National Standardization Council of Thailand

CALIBRATION REPORT

Professional Calibration & Services Co., Ltd.

Certificate No.: EL41650/24

Page : 3 of 3

Calibration Results

Sound Pressure Level Accuracy

Nominal Value	Measured Value	UUC Error	Uncertainty (±)
94 dB	93.97 dB	0.03 dB	0.17 dB
114 dB	114.30 dB	-0.30 dB	0.17 dB

...End...



ADVANTAGE CENTER CO., LTD.

59/494 M.6, Frakham Road, T.Kukhot, Lumlookkar, Pathumthani 12130 Thailand.

Tel. (66-2) 9873248-50 Fax: (66-2) 9873252 E-mail: info.accl2662@gmail.com

pornsak2008@yahoo.co.th



CALIBRATION LABORATORY

Certificate No. RA-2412024-1

Job No. RA-2412024

Certificate of Calibration

FOR

Equipment Name : Sound Level Meter

Manufacturer : Scarlet Tech

Model : ST11D

Serial Number : 820861

Customer Code : SLM-28

Location of Calibration : In Lab

Customer Name : Viridian Environmental Service Co., Ltd.

149/119 Moo 2, Krung Non-Chong Thanom Rd., Mahasawat, Bang Kruay, Nonthaburi 11130

Calibration Procedure : CPE-04-01

Received Date : Dec 13, 2024

Calibration Date : Dec 17, 2024

Recommended Due Date : N/A

CONDITION AS RECEIVED : Normal

Environmental Conditions

Ambient Temperature : $(25 \pm 2) ^\circ\text{C}$

Relative Humidity : $(50 \pm 15) \% \text{RH}$

Result : No Adjustment (See data attached in page 3 to the end of certificate)

1. The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%.
2. The Unit Under Calibration (UUC) has been calibrated by using the working standard which is traceable to SI-Units. The calibration procedure documented is intended to implement the requirements of ISO/IEC 17025 : 2017
3. The working standard is indicated in page 2 of this certificate.
4. This report applies to the item calibrated and shall not be reproduced except in full, without written approval by Calibration Laboratory, Advantage Center Co., Ltd.

Calibrated by : P. Noppadon

Approved by :


(Pornsak)

Date of Issue : Dec 18, 2024

Laboratory Management

Page 1 of 3

Certificate No.: RA-2412024-1

Reference Standards

Equipment Name	Serial No.	Certificate No.	Due Date	Traceability to
Sound Calibrator	170603302	EEL.BP. 32/1167	Nov 14, 2025	TISTR

Traceability

This calibration is traceable to the International System of Unit via :

- TISTR : Thailand Institute of Scientific and Technological Research



Certificate No. : RA-2412024-1

Result of Calibration

Calibration Range : 94 dB, 114 dB

Function : Measurement @ 1 kHz

Select A Fast response

STD Setting	UUC Reading (dB)	Correction (dB)	Uncertainty of Measurement (± dB)
94.42 dB	94.4	0.02	0.88
114.32 dB	114.3	0.02	0.88

Select A Slow response

STD Setting	UUC Reading (dB)	Correction (dB)	Uncertainty of Measurement (± dB)
94.42 dB	94.3	0.12	0.88
114.32 dB	114.4	-0.08	0.88

Select C Fast response

STD Setting	UUC Reading (dB)	Correction (dB)	Uncertainty of Measurement (± dB)
94.42 dB	94.3	0.12	0.88
114.32 dB	114.4	-0.08	0.88

Select C Slow response

STD Setting	UUC Reading (dB)	Correction (dB)	Uncertainty of Measurement (± dB)
94.42 dB	94.3	0.12	0.88
114.32 dB	114.3	0.02	0.88

STD = Standard

UUC = Unit Under Calibration

- End of Certificate -



CALIBRATION LABORATORY

Certificate No. RA-2412024-2

Job No. RA-2412024

Certificate of Calibration

FOR

Equipment Name : Sound Level Meter

Manufacturer : Scarlet Tech

Model : ST11D

Serial Number : 820862

Customer Code : SLM-29

Location of Calibration : In Lab

Customer Name : Viridian Environmental Service Co., Ltd.

149/119 Moo 2, Krung Non-Chong Thanom Rd., Mahasawat, Bang Kruay, Nonthaburi 11130

Calibration Procedure : CPE-04-01

Received Date : Dec 13, 2024

Calibration Date : Dec 17, 2024

Recommended Due Date : N/A

CONDITION AS RECEIVED : Normal

Environmental Conditions

Ambient Temperature : $(25 \pm 2) ^\circ\text{C}$

Relative Humidity : $(50 \pm 15) \% \text{RH}$

Result : No Adjustment (See data attached in page 3 to the end of certificate)

1. The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%.
2. The Unit Under Calibration (UUC) has been calibrated by using the working standard which is traceable to SI-Units. The calibration procedure documented is intended to implement the requirements of ISO/IEC 17025 : 2017
3. The working standard is indicated in page 2 of this certificate.
4. This report applies to the item calibrated and shall not be reproduced except in full, without written approval by Calibration Laboratory, Advantage Center Co., Ltd.

Calibrated by : P. Noppadon

Approved by :


(Pomsak S.)

Date of Issue : Dec 18, 2024

Laboratory Management

Certificate No.: RA-2412024-2

Reference Standards

Equipment Name	Serial No.	Certificate No.	Due Date	Traceability to
Sound Calibrator	170603302	EEL.BP. 32/1167	Nov 14, 2025	TISTR

Traceability

This calibration is traceable to the International System of Unit via ;

- TISTR : Thailand Institute of Scientific and Technological Research



Certificate No. : RA-2412024-2

Result of Calibration

Calibration Range : 94 dB, 114 dB

Function : Mesurement @ 1 kHz

Select A Fast response

STD Setting	UUC Reading (dB)	Correction (dB)	Uncertainty of Measurement (± dB)
94.42 dB	94.4	0.02	0.88
114.32 dB	114.3	0.02	0.88

Select A Slow response

STD Setting	UUC Reading (dB)	Correction (dB)	Uncertainty of Measurement (± dB)
94.42 dB	94.4	0.02	0.88
114.32 dB	114.3	0.02	0.88

Select C Fast response

STD Setting	UUC Reading (dB)	Correction (dB)	Uncertainty of Measurement (± dB)
94.42 dB	94.3	0.12	0.88
114.32 dB	114.3	0.02	0.88

Select C Slow response

STD Setting	UUC Reading (dB)	Correction (dB)	Uncertainty of Measurement (± dB)
94.42 dB	94.3	0.12	0.88
114.32 dB	114.3	0.02	0.88

STD = Standard

UUC = Unit Under Calibration

- End of Certificate -



ภาคผนวกที่ 5-3
เอกสารสอบเทียบเครื่องมือตรวจวัดความสั่นสะเทือน



CALIBRATION LABORATORY Co., LTD.

2/10-11,14, 55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



CERTIFICATE OF CALIBRATION

FOR

NOMENCLATURE : VIBRATION METER
MANUFACTURER : INSTANTEL
MODEL / TYPE : 721A2501/721A2901
SERIAL NO. : UM13202/UM13202
CLID. NO. : 252102517
JOB CONTROL NO. : 241219135224
CALIBRATION SERVICE : ☒ IN-LABORATORY ☐ ON-SITE

CUSTOMER : PACIFIC LABORATORY CO., LTD.
14/5358 MOO 14 TAMBOL BANG BUA THONG
AMPHOE BANG BUA THONG NONTHABURI 11110

DATE OF RECEIVED : 19 December 2024

DATE OF ISSUED : 23 December 2024

The report of calibration shall not be reproduced except in full without approval of the Calibration Laboratory Co., Ltd.

Calibrated By :

Suwit Phuanbusabong
Calibration Engineer

Approved By :

Mongk
Authorized Signatory
23 December 2024



This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to the
International System of Units (SI)

Certificate No. Q24135224

F3-011-05/12-23

page 1 of 2



@clccalibration



CALIBRATION LABORATORY Co., LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



REPORT OF CALIBRATION

FOR

NOMENCLATURE	:	VIBRATION METER
MANUFACTURER	:	INSTANTEL
MODEL / TYPE	:	721A2501/721A2901
SERIAL NO.	:	UM13202/UM13202
DATE OF CALIBRATION	:	20 December 2024

ENVIRONMENT CONDITIONS :

Temperature : $(23 \pm 2) ^\circ\text{C}$

Relative Humidity : $(55 \pm 15) \% \text{RH}$

PROCEDURE USED :

This instrument was calibrated under procedure No. **CLC-CPEE-08** based on **ISO 16063-21** as calibration guideline.

The calibration was performed by using Digital Multimeter, Programmable Timer/Counter, Vibration Calibrator which maintained by the Calibration Laboratory Co., Ltd.

REFERENCE STANDARD USED :

1. Vibration Calibrator, The Modal Shop Model 9110D S/N. 11424.
2. Programmable Timer/Counter, Philips Model PM6680B S/N. SM607101.
3. Digital Multimeter, Keysight Technologies Model 3458A S/N. MY59352733.

TRACEABILITY :

1. The measurements are traceable to International System of Units (SI), through National Institute of Metrology (Thailand) Certificate No. AV-0030-24, Due Date 19 July 2025.
2. The measurements are traceable to International System of Units (SI), through Aeronautical Radio of Thailand Ltd. Certificate No. 07-0050/24, Due Date 13 May 2025.
3. The measurements are traceable to International System of Units (SI), through National Institute of Metrology (Thailand) Certificate No. EE-0060-24, Due Date 26 June 2025.

UNCERTAINTY :

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor $k = 2,00$ which for a normal distribution corresponds to a coverage probability of approximately 95 %. It has been evaluated according to the "Evaluation of the Uncertainty of Measurement in Calibration (EA-4/02 M:2022)"

Certificate No. Q24135224

F3-011-05/12-23

page 2 of 3



@clccalibration



CALIBRATION LABORATORY Co., LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



CONDITION OF CALIBRATION ITEM : RECEIVED IN GOOD OPERATIONAL CONDITION

MEASUREMENT RESULTS : (X) without adjustment () adjustment

CALIBRATION DATA

VELOCITY RESULT

Test point		Mode	STD Reading	DUC Reading	Correction	Uncertainty
(mm/s)	(frequency)		(mm/s)	(mm/s)	(mm/s)	\pm (% of rdg.)
10	160 Hz	peak	10.000	10.324	-0.324	1.5
20	160 Hz		20.000	20.388	-0.388	1.5
30	160 Hz		30.000	30.465	-0.465	1.5
40	160 Hz		40.000	40.572	-0.572	1.5
50	160 Hz		50.000	50.689	-0.689	1.5

Note. The Scope of Accredited ANAB Certificate No. ACDM-2814 Version 012 Page 2 of 67

This report is valid for the above stated instrument/s only.

End of Certificate

Certificate No. Q24135224

F3-011-05/12-23

page 3 of 3



@clccalibration

ภาคผนวกที่ 5-4

เอกสารสอบเทียบเครื่องมือตรวจวิเคราะห์คุณภาพน้ำ

CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhaprachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech.cal@yahoo.com, calibratech.cal@hotmail.com



Certificate of Calibration

Certificate No. : 67-420078-1

Page : 1 of 2

Submitted by : Pacific Laboratory Co., Ltd.

14/5358 Moo 14, T. Bang Bua Thong, A. Bang Bua Thong, Nonthaburi 11110 Thailand

Equipment : pH Meter with electrode

pH meter

Manufacturer : Eutech

Model : pH 700

Range : N/A

pH

Resolution : 0.01 pH

Serial No. : 2841305

ID No. : LAB-PH-002

Electrode

Model : N/A

Serial No. : 3172493

Environment : On site calibration was carried out at the Laboratory, Pacific Laboratory Co., Ltd

Ambient Temperature : (25.0 to 26.0) °C

Relative Humidity : (40 to 45) %

Date of Received : 30 July 2024

Date of Calibration : 30 July 2024

Date of Issue : 03 August 2024

Calibrated by : Permpoon Chanpu

Calibration Method : In-house method CAL-M4201 direct measurement by using standard voltage calibrator and using certified reference material (CRM)

Reference Standard Instruments : This certification is traceable to the International System of Units

1. Multiproduct Calibrator

ID No.	Cert. No.	Due Date	Traceability
400005	SG-E-00307/66	23 Aug 2025	National Institute of Metrology Thailand (NIMT)

2. Standard Buffer Solution

pH	Cert. No.	Lot No.	Exp. Date	Traceability
4.008	61293328	986281	25 Apr 2026	CPA Chem Ltd. Accredited to ISO 17034 and ISO/IEC 17025
6.986	61281486	986283	25 Apr 2025	CPA Chem Ltd. Accredited to ISO 17034 and ISO/IEC 17025
9.997	61281073	986282	25 Apr 2025	CPA Chem Ltd. Accredited to ISO 17034 and ISO/IEC 17025

Approved by :

(Signature)

Laboratory Manager

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhaprachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech.cal@yahoo.com, calibratech.cal@hotmail.com

Certificate of Calibration

Certificate No. : 67-420078-1

Page : 2 of 2

Result of Calibration :

UUC Condition As-Received : Good

Function : Electrical measurement
pH meter

Performing standard curve by Multiproduct Calibrator at pH (4,7,10)

Adjustment Curve at nominal pH	Applied Voltage (mV)	Nominal Value (pH)	UUC Reading		Correction (mV)	Uncertainty (± mV)
			(pH)	(mV)		
4, 7, 10	177.4800	4	4.00	177.5	0.0	0.12
	0.0000	7	7.00	0.1	-0.1	0.086
	-177.4800	10	10.00	-177.4	-0.1	0.12

Function : pH meter with electrode

Performing a three - buffer standard curve using buffer nominal pH (4,7,10)

Adjustment Curve at nominal pH	Standard Buffer (pH)	UUC Reading (pH)	Correction (pH)	Uncertainty (± pH)
4, 7, 10	4.008	4.01	0.00	0.0097
	6.986	7.00	-0.01	0.011
	9.997	10.01	-0.01	0.014

Remark

UUC : Unit Under Calibration

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

- 000 -



CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhprachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech.cal@yahoo.com, calibratech.cal@hotmail.com



NSC-TISI-TIS17025
CALIBRATION 0030

Certificate of Calibration

Certificate No. : 67-420078-2

Page : 1 of 2

Submitted by : Pacific Laboratory Co., Ltd.

14/5358 Moo 14, T. Bang Bua Thong, A. Bang Bua Thong, Nonthaburi 11110 Thailand

Equipment : pH Meter with electrode

pH meter

Manufacturer : Eutech

Model : pH 700

Range : N/A

pH

Resolution : 0.01 pH

Serial No. : 2841305

ID No. : LAB-PH-002

Electrode

Model : N/A

Serial No. : 3052953

Environment : On site calibration was carried out at the Laboratory, Pacific Laboratory Co., Ltd

Ambient Temperature : (25.0 to 26.0)^o C

Relative Humidity : (40 to 45) %

Date of Received : 30 July 2024

Date of Calibration : 30 July 2024

Date of Issue : 03 August 2024

Calibrated by : Permpon Chanpu

Calibration Method : In-house method CAL-M4201 direct measurement by using standard voltage calibrator and using certified reference material (CRM)

Reference Standard Instruments : This certification is traceable to the International System of Units

1. Multiproduct Calibrator

ID No.	Cert. No.	Due Date	Traceability
400005	SG-E-00307/66	23 Aug 2025	National Institute of Metrology Thailand (NIMT)

2. Standard Buffer Solution

pH	Cert. No.	Lot No.	Exp. Date	Traceability
4.008	61293328	986281	25 Apr 2026	CPA Chem Ltd. Accredited to ISO 17034 and ISO/IEC 17025
6.986	61281486	986283	25 Apr 2025	CPA Chem Ltd. Accredited to ISO 17034 and ISO/IEC 17025
9.997	61281073	986282	25 Apr 2025	CPA Chem Ltd. Accredited to ISO 17034 and ISO/IEC 17025

Approved by :

(Sur

Laboratory Manager

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.

CAL-F0031-03



CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhaprachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech.cal@yahoo.com, calibratech.cal@hotmail.com

Certificate of Calibration

Certificate No. : 67-420078-2

Page : 2 of 2

Result of Calibration :

UUC Condition As-Received : Good

Function : Electrical measurement

pH meter

Performing standard curve by Multiproduct Calibrator at pH (4,7,10)

Adjustment Curve at nominal pH	Applied Voltage (mV)	Nominal Value (pH)	UUC Reading		Correction (mV)	Uncertainty (± mV)
			(pH)	(mV)		
4, 7, 10	177.4800	4	4.00	177.5	0.0	0.12
	0.0000	7	7.00	0.1	-0.1	0.086
	-177.4800	10	10.00	-177.4	-0.1	0.12

Function : pH meter with electrode

Performing a three - buffer standard curve using buffer nominal pH (4,7,10)

Adjustment Curve at nominal pH	Standard Buffer (pH)	UUC Reading (pH)	Correction (pH)	Uncertainty (± pH)
4, 7, 10	4.008	4.01	0.00	0.0097
	6.986	7.00	-0.01	0.011
	9.997	10.01	-0.01	0.014

Remark

UUC : Unit Under Calibration

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

- ๐0๐ -



CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhaphrachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech.cal@yahoo.com, calibratech.cal@hotmail.com



Certificate of Calibration

Certificate No. : 67-400424-1

Page : 1 of 2

Submitted by : Pacific Laboratory Co., Ltd
14/5358 Moo 14, T. Bang Bua Thong, A. Bang Bua Thong, Nonthaburi 11110 Thailand

Equipment : Digital Thermometer with Thermistor probe
Temperature Indicator

Manufacturer : Eutech Model : pH 700
Range : N/A °C Resolution : 0.1 °C
Serial No. : 2841305 ID No. : LAB-PH-002

Thermistor probe
Model : N/A Sheath Material : Stainless
Diameter : 3 mm. Length : 115 mm.
Serial No. : PHSTEMB01P 304 ID No. : LAB-PH-002

Environment : On site calibration was carried out at the Laboratory, Pacific Laboratory Co., Ltd

Ambient Temperature : (25.0 to 25.6) °C
Relative Humidity : (45 to 47) %
Line Voltage : (220.0 to 222.0) VAC

Date of Received : 30 July 2024

Date of Calibration : 30 July 2024

Date of Issue : 03 August 2024

Calibrated by : Permpon Chanpu

Calibration Method : This instrument was calibrated by In-house method comparison technique CAL-M4003 by compared with PRT in the liquid bath at the constant controlled temperature.

The temperature scale used was based on ITS-90

Reference Standard Instruments : This certification is traceable to the International System of Units

1. Platinum Resistance Thermometer (PRT)

ID No.	Cert. No.	Due Date	Traceability
400002	TT-0074-22	23 Aug 2025	National Institute of Metrology Thailand (NIMT)

2. Standard Digital Thermometer

ID No.	Cert. No.	Due Date	Traceability
400033	22E569	25 Apr 2025	National Institute of Metrology Thailand (NIMT)

Approved by :

(Bu

Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.

CAL-F0031-03



CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhaprachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech_cal@yahoo.com, calibratech_cal@hotmail.com

Certificate of Calibration

Certificate No. : 67-400424-1

Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Function : Temperature measurement

Immersion Depth (mm.)	Standard Reading (°C)	UUC Reading (°C)	Correction (°C)	Uncertainty (± °C)
115	25.005	24.8	0.2	0.19

Remark

UUC : Unit Under Calibration

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$,

providing a level of confidence of approximately 95%

- 000 -



CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhaphrachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech.cal@yahoo.com, calibratech.cal@hotmail.com



NSG-TISI-TIS 17025
CALIBRATION 0030

Certificate of Calibration

Certificate No. : 67-400454-3

Page : 1 of 2

Submitted by : Pacific Laboratory Co., Ltd

14/5358 Moo 14, T. Bang Bua Thong, A. Bang Bua Thong, Nonthaburi 11110 Thailand

Equipment : Temperature controlled enclosure (Incubator)

Manufacturer : Aqua Lytic

Model : TC 135S

Range : N/A °C

Resolution : 0.1 °C

Serial No. : 0614/000033

ID No. : LAB-IB-001

Environment : On site calibration was carried out at the Laboratory, Pacific Laboratory Co., Ltd

Ambient Temperature : (25.5 to 26.0) °C

Relative Humidity : (40 to 45) %

Line Voltage : (220.0 to 222.0) V

Date of Received : 30 July 2024

Date of Calibration : 30 July 2024

Date of Issue : 03 August 2024

Calibrated by : Permpoon Chanpu

Calibration Method : CAL-M4004, TLAS G-20

The temperature scale used was based on ITS-90

Reference Standard Instruments : This certification is traceable to the International System of Units
Standard Digital Thermometer with RTD Probe

<u>ID No.</u>	<u>Cert. No.</u>	<u>Due Date</u>	<u>Traceability</u>
400029 & 400043	67-400245-1	27 Oct 2024	National Institute of Metrology Thailand (NIMT)

Approved by :



Laboratory Manager

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



CAL-F0031-03

CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhaprachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech.cal@yahoo.com, calibratech.cal@hotmail.com

Certificate of Calibration

Certificate No. : 67-400454-3


Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Function : Temperature measurement

This instrument was setting air ventilation at position 0 (close)

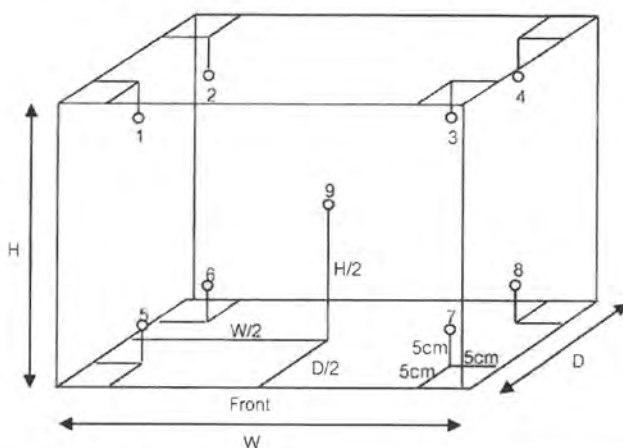

Inside of Chamber

W = 0.51 m

D = 0.04 m

H = 0.70 m

Capacity = 0.02 m³

Test Point (" C)	Setting Temperature (" C)	Indicating Temperature (" C)	Measured Temperature (" C) @ Sensor No.									Uncertainty (± " C)
			1	2	3	4	5	6	7	8	9	
20.0	20.5	20.5	20.07	19.92	19.95	19.93	19.93	19.92	19.92	19.96	19.88	0.67

Test Point (" C)	Setting Temperature (" C)	Indicating Temperature (" C)	Measured Uniformity (" C)	Measured Stability (" C)	Overall Variation (" C)
20.0	20.5	20.5	0.41	0.33	0.70

Remark The uncertainty is not combine uniformity of the air chamber

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k = 2 ,
providing a level of confidence of approximately 95%

- o0o -



CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhaphrachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech.cal@yahoo.com, calibratech.cal@hotmail.com



NSC-TISI-TIS 17025
CALIBRATION 0030

Certificate of Calibration

Certificate No. : 67-400454-2

Page : 1 of 2

Submitted by : Pacific Laboratory Co., Ltd
14/5358 Moo 14, T. Bang Bua Thong, A. Bang Bua Thong, Nonthaburi 11110 Thailand

Equipment : Water Bath
Manufacturer : Memmert
Range : N/A °C
Serial No. : L514.0184
Model : WNB 22
Resolution : 0.1 °C
ID No. : LAB-WB-001

Environment : On site calibration was carried out at the Laboratory, Pacific Laboratory Co., Ltd
Ambient Temperature : (30.0 to 31.3) °C
Relative Humidity : (60 to 65) %
Line Voltage : (220.0 to 222.0) V

Date of Received : 30 July 2024

Date of Calibration : 30 July 2024

Date of Issue : 03 August 2024

Calibrated by : Pernnpon Chanpu

Calibration Method : This instrument was calibrated by In-house method CAL-M4006 based on ASTM E715-80
The temperature scale used was based on ITS-90

Reference Standard Instruments : This certification is traceable to the International System of Units
Standard Digital Thermometer with RTD probe

<u>ID No.</u>	<u>Cert. No.</u>	<u>Due Date</u>	<u>Traceability</u>
400029 & 400031	67-400244-1	24 Oct 2024	National Institute of Metrology Thailand (NIMT)

Approved by :

(Surach

Laboratory Manager

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhprachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech.cal@yahoo.com, calibratech.cal@hotmail.com

Certificate of Calibration


Certificate No. : 67-400454-2

Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Function : Temperature measurement

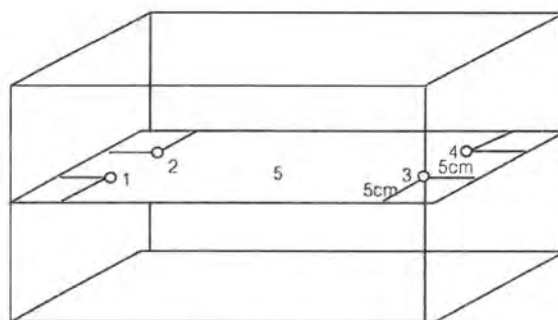

Front

Test Point (" C)	Setting Temperature (" C)	Indicating Temperature (" C)	Measured Temperature (" C) @ Sensor No.					Uncertainty (± " C)	Measured Uniformity (" C)	Measured Stability (" C)
			1	2	3	4	5			
65.0	65.0	65.0	64.61	64.70	64.66	64.64	64.68	0.18	0.12	0.05
95.0	95.0	95.0	94.60	94.69	94.70	94.61	94.70	0.18	0.15	0.03

Remark The uncertainty is not combine uniformity of the water bath

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

- o0o -



CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhprachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech.cal@yahoo.com, calibratech.cal@hotmail.com



NSC-TISI-TIS17025
CALIBRATION 0030

Certificate of Calibration

Certificate No. : 67-400454-1

Page : 1 of 2

Submitted by : Pacific Laboratory Co., Ltd

14/5358 Moo 14, T. Bang Bua Thong, A. Bang Bua Thong, Nonthaburi 11110 Thailand

Equipment : Temperature controlled enclosure (Oven)

Manufacturer : Memmert

Model : UN 55

Range : N/A °C

Resolution : 0.1 °C

Serial No. : B214.1879

ID No. : LAB-OV-001

Environment : On site calibration was carried out at the Laboratory, Pacific Laboratory Co., Ltd

Ambient Temperature : (30.0 to 31.3) °C

Relative Humidity : (60 to 65) %

Line Voltage : (220.0 to 222.0) V

Date of Received : 30 July 2024

Date of Calibration : 30 July 2024

Date of Issue : 03 August 2024

Calibrated by : Permpon Chanpu

Calibration Method : CAL-M4004, TLAS G-20

The temperature scale used was based on ITS-90

Reference Standard Instruments : This certification is traceable to the International System of Units
Standard Digital Thermometer with Thermocouple probe

<u>ID No.</u>	<u>Cert. No.</u>	<u>Due Date</u>	<u>Traceability</u>
400029 & 400030	67-400246-1	25 Oct 2024	National Institute of Metrology Thailand (NIMT)

Approved by :

(Sura

Laboratory Manager

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.

CAL-F0031-03



CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhaprachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech.cal@yahoo.com, calibratech.cal@hotmail.com

Certificate of Calibration

Certificate No. : 67-400454-1


Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Function : Temperature measurement

This instrument was setting air ventilation at position 0 (close)

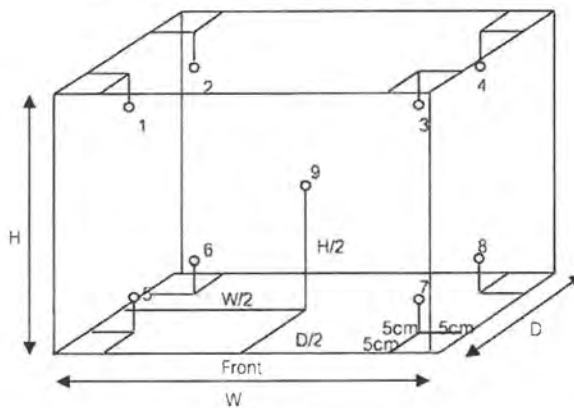

Inside of Chamber

W = 0.40 m

D = 0.33 m

H = 0.40 m

Capacity = 0.05 m³

Test Point (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Temperature (°C) @ Sensor No.									Uncertainty (± °C)
			1	2	3	4	5	6	7	8	9	
104.0	107.0	107.0	105.1	104.9	104.8	104.8	102.9	103.6	103.7	104.1	103.9	0.84
180.0	184.0	184.0	180.5	180.5	180.3	179.7	176.8	177.2	178.1	181.2	179.5	1.4

Test Point (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Uniformity (°C)	Measured Stability (°C)	Overall Variation (°C)
104.0	107.0	107.0	1.4	0.4	2.5
180.0	184.0	184.0	3.3	0.7	5.6

Remark The uncertainty is not combine uniformity of the air chamber

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

- o0o -

