

ภาคผนวก ค

ใบรับรองผลการตรวจวัดคุณภาพสิ่งแวดล้อม

ภาคผนวก ค-1

ผลการตรวจวัดสารโพรพิลีนออกไซด์ บริเวณพื้นที่ถังปฏิกิริยา



Analysis / Test Report

Client : Dow Chemical Thailand Ltd.

10 Moo 2, Asia Industrial Estate, Tambol Banchang, Amphur Banchang, Rayong
Thailand 21130

P/O : 4516938776

Project Name : Environmental Quality Monitoring

Project Location : AIE_PG Plant

Lot ID: 24143144

Date Received : Jan 10, 2025

Date Reported : Jan 16, 2025

Report Number : 3199903-1

Page 1 of 1

Sample Number 24143144-1
Sampled Date Jan 10, 2025
Sample Description Air Quality
Location บริเวณพื้นที่ดังปฎิบัติ
Date Analysis Commenced Jan 11, 2025
Condition of Sample Drawn into one sorbent tube, refrigerated
Barometric Pressure 755 mmHg
Atmospheric Temperature 28.4 °C

Analyte	Sampled Date/time	Unit	LOD	LOQ (LOR)	Result	Guideline Limit	Method	Guideline	Testing Location
Air Testing									
Propylene Oxide	10:00 AM - 12:00 PM	ppm	-	0.10	<0.10	100	NIOSH (1994), 1612	MOL	Bangkok

Guideline :

MOL : Announcement of the Department of Labour Protection and Welfare on Threshold Limit Values of Hazardous Chemical Substances Dated August 3, B.E. 2560 (2017)

Sampled By : Anurak Tongkhajonsakda

Remark :

- LOD : Limit of Detection
- "<" : Lower than LOQ (Limit of Quantitation) / LOR (Limit of Reporting)

Approved by

Orawan R.

Orawan Rakyong

Scientist (3)

Results apply to the sample(s) as submitted, unless the sampling was conducted by ALS. No part of this report may be reproduced in any form without written consent from the laboratory. ALS Laboratory Group (Thailand) strongly recommends that this report is not reproduced except in full.

ADDRESS 104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan, Khet Suan Luang, Bangkok 10250 Thailand | PHONE +66 0 2760 3000 | FAX +66 0 2760 3197
ALS LABORATORY GROUP (THAILAND) CO., LTD. An ALS Limited Company

Life Sciences

www.alsglobal.com

RIGHT SOLUTIONS RIGHT PARTNER

8525-41/ EMAIL



Analysis / Test Report

Client : Dow Chemical Thailand Ltd.

10 Moo 2, Asia Industrial Estate, Tambol Banchang, Amphur Banchang, Rayong
Thailand 21130

P/O : 4516938776

Project Name : Environmental Quality Monitoring

Project Location : AIE_PG Plant

Lot ID: 253571

Date Received : Feb 11, 2025

Date Reported : Feb 20, 2025

Report Number : 3211553-1

Page 1 of 1

Sample Number 253571-1
Sampled Date Feb 10, 2025
Sample Description Air Quality
Location บริเวณพื้นที่ตั้งปฏิกิริยา
Date Analysis Commenced Feb 13, 2025
Condition of Sample Drawn into one sorbent tube, refrigerated
Barometric Pressure 754 mmHg
Atmospheric Temperature 28.6 °C

Analyte	Sampled Date/time	Unit	LOD	LOQ (LOR)	Result	Guideline Limit	Method	Guideline	Testing Location
Air Testing									
Propylene Oxide	09:30 AM - 11:30 AM	ppm	-	0.10	<0.10	100	NIOSH (1994), 1612	MOL	Bangkok

Guideline :

MOL : Announcement of the Department of Labour Protection and Welfare on Threshold Limit Values of Hazardous Chemical Substances Dated August 3, B.E. 2560 (2017)

Sampled By : Tarin Octjinda

Remark :

- LOD : Limit of Detection
- "<" : Lower than LOQ (Limit of Quantitation) / LOR (Limit of Reporting)

Approved by

Orawan R.

Orawan Rakyong

Scientist (3)

Results apply to the sample(s) as submitted, unless the sampling was conducted by ALS. The report shall not be reproduced except in full without the written approval of the laboratory.



Analysis / Test Report

Client : Dow Chemical Thailand Ltd.
10 Moo 2, Asia Industrial Estate, Tambol Banchang, Amphur Banchang, Rayong
Thailand 21130
P/O : 4516938776
Project Name : Environmental Quality Monitoring
Project Location : AIE_PG Plant

Lot ID: 2529511

Date Received : Apr 21, 2025
Date Reported : Apr 28, 2025
Report Number : 3268540-1

Page 1 of 1

Sample Number 2529511-1
Sampled Date Apr 18, 2025
Sample Description Air Quality
Location บริเวณพื้นที่ตั้งปฏิกิริยา
Date Analysis Commenced Apr 22, 2025
Condition of Sample Drawn into one sorbent tube, refrigerated
Barometric Pressure 756 mmHg
Atmospheric Temperature 30.8 °C

Analyte	Sampled Date/time	Unit	LOD	LOQ (LOR)	Result	Guideline Limit	Method	Guideline	Testing Location
Air Testing									
Propylene Oxide	02:05 PM - 04:05 PM	ppm	-	0.10	<0.10	100	NIOSH (1994), 1612	MOL	Bangkok

Guideline :

MOL : Announcement of the Department of Labour Protection and Welfare on Threshold Limit Values of Hazardous Chemical Substances Dated August 3, B.E. 2560 (2017)

Sampled By : Apisit Singha

Remark :

- LOD : Limit of Detection
- "<" : Lower than LOQ (Limit of Quantitation) / LOR (Limit of Reporting)

Approved by

Orawan R.

Orawan Rakyong
Scientist (3)

Results apply to the sample(s) as submitted, unless the sampling was conducted by ALS. The report shall not be reproduced except in full without the written approval of the laboratory.



Analysis / Test Report

Client : Dow Chemical Thailand Ltd.
10 Moo 2, Asia Industrial Estate, Tambol Banchang, Amphur Banchang, Rayong
Thailand 21130
P/O : 4516938776
Project Name : Environmental Quality Monitoring
Project Location : AIE_PG Plant

Lot ID: 2540909

Date Received : May 07, 2025
Date Reported : May 16, 2025
Report Number : 3295291-1

Page 1 of 1

Sample Number 2540909-1
Sampled Date May 06, 2025
Sample Description Air Quality
Location บริเวณพื้นที่ตั้งปฏิกิริยา
Date Analysis Commenced May 10, 2025
Condition of Sample Drawn into one 10-L air sampling bag
Barometric Pressure 756 mmHg
Atmospheric Temperature 31.0 °C

Analyte	Sampled Date/time	Unit	LOD	LOQ (LOR)	Result	Guideline Limit	Method	Guideline	Testing Location
Air Testing									
Propylene Oxide	10:00 AM - 12:00 PM	ppm	-	0.10	<0.10	100	NIOSH (1994), 1612	MOL	Bangkok

Guideline :

MOL : Announcement of the Department of Labour Protection and Welfare on Threshold Limit Values of Hazardous Chemical Substances Dated August 3, B.E. 2560 (2017)

Sampled By : Norranon Tathongkham

Remark :

- LOD : Limit of Detection
- "<" : Lower than LOQ (Limit of Quantitation) / LOR (Limit of Reporting)

Approved by

Orawan R.

Orawan Rakyong
Scientist (3)

Results apply to the sample(s) as submitted, unless the sampling was conducted by ALS. The report shall not be reproduced except in full without the written approval of the laboratory.



Analysis / Test Report

Client : Dow Chemical Thailand Ltd.
10 Moo 2, Asia Industrial Estate, Tambol Banchang, Amphur Banchang, Rayong
Thailand 21130
P/O : 4516938776
Project Name : Environmental Quality Monitoring
Project Location : AIE_PG Plant

Lot ID: 2549585

Date Received : Jun 06, 2025
Date Reported : Jun 13, 2025
Report Number : 3316059-1

Page 1 of 1

Sample Number 2549585-1
Sampled Date Jun 06, 2025
Sample Description Air Quality
Location บริเวณพื้นที่ดังปฏิกิริยา
Date Analysis Commenced Jun 07, 2025
Condition of Sample Drawn into one sorbent tube, refrigerated
Barometric Pressure 752 mmHg
Atmospheric Temperature 33.2 °C

Analyte	Sampled Date/time	Unit	LOD	LOQ (LOR)	Result	Guideline Limit	Method	Guideline	Testing Location
Air Testing									
Propylene Oxide	09:45 AM - 11:45 AM	ppm	-	0.10	<0.10	100	NIOSH (1994), 1612	MOL	Bangkok

Guideline :

MOL : Announcement of the Department of Labour Protection and Welfare on Threshold Limit Values of Hazardous Chemical Substances Dated August 3, B.E. 2560 (2017)

Sampled By : Tarin Octjinda

Remark :

- LOD : Limit of Detection
- "<" : Lower than LOQ (Limit of Quantitation) / LOR (Limit of Reporting)

Approved by

Saranya C.

Saranya Chalermthamrong
Scientist (4)

Results apply to the sample(s) as submitted, unless the sampling was conducted by ALS. The report shall not be reproduced except in full without the written approval of the laboratory.

ภาคผนวก ค-2

ผลการตรวจวัดระดับเสียงโดยทั่วไปบริเวณชุมชน
ที่อยู่ใกล้เคียงพื้นที่โครงการ



Analysis / Test Report

TESTING
No.0042

Client : Dow Chemical Thailand Ltd.

10 Moo 2, Asia Industrial Estate, Tambol Banchang, Amphur Banchang, Rayong Thailand 21130

P/O : 4516938776

Project Name : Environmental Quality Monitoring

Project Location : AIE_PG Plant

Lot ID: 2518560

Date Received : May 06, 2025

Date Reported : May 13, 2025

Report Number: 3303639-1

Page 1 of 1

Sample Number 2518560-1
Parameter Noise (Leq 24 hrs.)
Location กลุ่มบ้านประทุมมิตร (ที่อยู่ใกล้พื้นที่โครงการมากที่สุด) (GPS 47P 0726338, 1405748)
Measurement Date Apr 28 - Apr 29, 2025
Measurement by Sitpawit Suwannarat
Sound Level meter Serial No. 1173610

Time	Leq (dB(A))	Lmax (dB(A))	L90 (dB(A))
11:00 AM - 12:00 PM	52.9	88.3	45.0
12:00 PM - 01:00 PM	52.3	76.3	45.9
01:00 PM - 02:00 PM	51.6	73.1	46.2
02:00 PM - 03:00 PM	52.9	82.2	45.7
03:00 PM - 04:00 PM	56.8	88.4	45.1
04:00 PM - 05:00 PM	53.6	74.9	45.8
05:00 PM - 06:00 PM	54.3	76.4	45.4
06:00 PM - 07:00 PM	58.1	90.3	44.6
07:00 PM - 08:00 PM	54.2	78.0	46.2
08:00 PM - 09:00 PM	50.0	77.1	46.4
09:00 PM - 10:00 PM	47.9	66.6	45.8
10:00 PM - 11:00 PM	49.9	72.7	46.7
11:00 PM - 12:00 AM	47.7	62.3	46.1
12:00 AM - 01:00 AM	46.4	59.2	45.2
01:00 AM - 02:00 AM	44.5	59.3	41.5
02:00 AM - 03:00 AM	42.2	62.5	40.1
03:00 AM - 04:00 AM	49.8	81.7	40.9
04:00 AM - 05:00 AM	44.5	63.8	39.8
05:00 AM - 06:00 AM	47.2	69.2	41.0
06:00 AM - 07:00 AM	52.6	80.9	45.2
07:00 AM - 08:00 AM	54.9	79.5	47.4
08:00 AM - 09:00 AM	59.0	89.4	45.0
09:00 AM - 10:00 AM	56.2	87.5	41.3
10:00 AM - 11:00 AM	52.3	80.1	44.3

Leq Average 24 hrs. (dB(A)) 53.2
Lmax (dB(A)) 90.3
L90 (dB(A)) 45.2
Ldn (dB(A)) 56.4
Standard (dB(A)) 70 115

Reference Method : ISO1996-1 and 1996-2

Standard : 1. ประกาศคณะกรรมการสิ่งแวดล้อมแห่งชาติ ฉบับที่ 15 (พ.ศ. 2540) เรื่องกำหนดมาตรฐานระดับเสียงโดยทั่วไป
2. ประกาศกระทรวงอุตสาหกรรม เรื่องกำหนดค่าระดับเสียงการรบกวน และระดับเสียงที่เกิดจากการประกอบกิจการโรงงาน พ.ศ. 2548

Remark : The laboratory has been accepted as an accredited laboratory complying with the ISO/IEC 17025.

Technical Management

Chontichak

Chonticha Subongkoch
Scientist (3)

Approved by

Supot S

Supot Salamteh
Section Head

ADDRESS 616/10 Moo 5 T. Maenam Khu A. Pluakdaeng Rayong 21140 Thailand | PHONE +66 0 3304 8555 | FAX +66 0 3304 8556
ALS LABORATORY GROUP (THAILAND) CO., LTD. An ALS Limited Company

Life Sciences

www.alsglobal.com

RIGHT SOLUTIONS RIGHT PARTNER



Analysis / Test Report

TESTING
No.0042

Client : Dow Chemical Thailand Ltd.
10 Moo 2, Asia Industrial Estate, Tambol Banchang, Amphur Banchang, Rayong Thailand 21130
P/O : 4516938776
Project Name : Environmental Quality Monitoring
Project Location : AIE_PG Plant

Lot ID: 2518560

Date Received : May 06, 2025
Date Reported : May 13, 2025
Report Number: 3303640-1

Page 1 of 1

Sample Number 2518560-2
Parameter Noise (Leq 24 hrs.)
Location กลุ่มบ้านประทุมมิตร (ที่อยู่ใกล้พื้นที่โครงการมากที่สุด) (GPS 47P 0726338, 1405748)
Measurement Date Apr 29 - Apr 30, 2025
Measurement by Sitpawit Suwannarat
Sound Level meter Serial No. 1173610

Time	Leq (dB(A))	Lmax (dB(A))	L90 (dB(A))
11:00 AM - 12:00 PM	51.9	75.3	43.1
12:00 PM - 01:00 PM	53.3	80.4	41.9
01:00 PM - 02:00 PM	51.3	72.0	40.5
02:00 PM - 03:00 PM	50.9	77.9	42.3
03:00 PM - 04:00 PM	49.6	72.3	44.2
04:00 PM - 05:00 PM	52.5	84.1	44.3
05:00 PM - 06:00 PM	52.7	79.3	44.2
06:00 PM - 07:00 PM	50.8	70.6	43.9
07:00 PM - 08:00 PM	53.7	72.6	48.7
08:00 PM - 09:00 PM	50.9	78.6	46.7
09:00 PM - 10:00 PM	48.0	66.9	45.8
10:00 PM - 11:00 PM	45.6	60.4	43.3
11:00 PM - 12:00 AM	53.6	86.3	43.4
12:00 AM - 01:00 AM	45.0	56.1	42.6
01:00 AM - 02:00 AM	45.4	67.4	43.3
02:00 AM - 03:00 AM	47.3	74.9	44.7
03:00 AM - 04:00 AM	46.0	70.4	41.7
04:00 AM - 05:00 AM	47.3	74.7	40.7
05:00 AM - 06:00 AM	52.3	78.4	42.5
06:00 AM - 07:00 AM	51.8	77.1	45.1
07:00 AM - 08:00 AM	55.9	79.0	45.8
08:00 AM - 09:00 AM	58.1	85.2	44.0
09:00 AM - 10:00 AM	49.4	73.1	40.9
10:00 AM - 11:00 AM	49.6	72.3	41.4

Leq Average 24 hrs. (dB(A)) 51.8
Lmax (dB(A)) 86.3
L90 (dB(A)) 43.3
Ldn (dB(A)) 56.5
Standard (dB(A)) 70 115

Reference Method : ISO1996-1 and 1996-2

Standard : 1. ประกาศคณะกรรมการสิ่งแวดล้อมแห่งชาติ ฉบับที่ 15 (พ.ศ. 2540) เรื่องกำหนดมาตรฐานระดับเสียงโดยทั่วไป
2. ประกาศกระทรวงอุตสาหกรรม เรื่องกำหนดค่าระดับเสียงการรบกวน และระดับเสียงที่เกิดจากการประกอบกิจการโรงงาน พ.ศ. 2548

Remark : The laboratory has been accepted as an accredited laboratory complying with the ISO/IEC 17025.

Technical Management

Chontichak

Chonticha Subongkoch
Scientist (3)

Approved by

Supot S

Supot Salamteh
Section Head

ADDRESS 616/10 Moo 5 T. Maenam Khu A. Pluakdaeng Rayong 21140 Thailand | PHONE +66 0 3304 8555 | FAX +66 0 3304 8556
ALS LABORATORY GROUP (THAILAND) CO., LTD. An ALS Limited Company

Life Sciences

www.alsglobal.com

RIGHT SOLUTIONS RIGHT PARTNER



Analysis / Test Report

TESTING
No.0042

Client : Dow Chemical Thailand Ltd.

10 Moo 2, Asia Industrial Estate, Tambol Banchang, Amphur Banchang, Rayong Thailand 21130

P/O : 4516938776

Project Name : Environmental Quality Monitoring

Project Location : AIE_PG Plant

Lot ID: 2518560

Date Received : May 06, 2025

Date Reported : May 13, 2025

Report Number: 3303641-1

Page 1 of 1

Sample Number 2518560-3
Parameter Noise (Leq 24 hrs.)
Location กลุ่มบ้านประทุมมิตร (ที่อยู่ใกล้พื้นที่โครงการมากที่สุด) (GPS 47P 0726338, 1405748)
Measurement Date Apr 30 - May 01, 2025
Measurement by Sitpawit Suwannarat
Sound Level meter Serial No. 1173610

Time	Leq (dB(A))	Lmax (dB(A))	L90 (dB(A))
11:00 AM - 12:00 PM	51.0	72.4	41.9
12:00 PM - 01:00 PM	51.9	74.3	42.8
01:00 PM - 02:00 PM	50.9	73.1	42.6
02:00 PM - 03:00 PM	53.3	83.6	44.5
03:00 PM - 04:00 PM	51.2	71.9	45.3
04:00 PM - 05:00 PM	52.2	76.7	43.4
05:00 PM - 06:00 PM	57.4	86.2	44.3
06:00 PM - 07:00 PM	58.9	87.5	44.3
07:00 PM - 08:00 PM	54.0	83.7	46.9
08:00 PM - 09:00 PM	53.2	75.7	47.7
09:00 PM - 10:00 PM	53.8	80.0	48.1
10:00 PM - 11:00 PM	60.6	88.1	47.9
11:00 PM - 12:00 AM	50.5	64.0	48.0
12:00 AM - 01:00 AM	48.9	71.8	46.8
01:00 AM - 02:00 AM	45.8	62.5	43.8
02:00 AM - 03:00 AM	45.7	66.1	43.4
03:00 AM - 04:00 AM	47.0	71.0	45.4
04:00 AM - 05:00 AM	48.5	62.0	46.5
05:00 AM - 06:00 AM	49.2	66.5	44.9
06:00 AM - 07:00 AM	52.7	73.5	44.4
07:00 AM - 08:00 AM	54.6	80.9	45.3
08:00 AM - 09:00 AM	52.6	79.5	40.8
09:00 AM - 10:00 AM	48.2	77.2	39.3
10:00 AM - 11:00 AM	52.5	79.2	43.1

Leq Average 24 hrs. (dB(A)) 53.6
Lmax (dB(A)) 88.1
L90 (dB(A)) 44.4
Ldn (dB(A)) 59.6
Standard (dB(A)) 70 115

Reference Method : ISO1996-1 and 1996-2

Standard : 1. ประกาศคณะกรรมการสิ่งแวดล้อมแห่งชาติ ฉบับที่ 15 (พ.ศ. 2540) เรื่องกำหนดมาตรฐานระดับเสียงโดยทั่วไป
2. ประกาศกระทรวงอุตสาหกรรม เรื่องกำหนดค่าระดับเสียงการรบกวน และระดับเสียงที่เกิดจากการประกอบกิจการโรงงาน พ.ศ. 2548

Remark : The laboratory has been accepted as an accredited laboratory complying with the ISO/IEC 17025.

Technical Management

Chontichak

Chonticha Subongkoch
Scientist (3)

Approved by

Supot S

Supot Salamteh
Section Head

ADDRESS 616/10 Moo 5 T. Maenam Khu A. Pluakdaeng Rayong 21140 Thailand | PHONE +66 0 3304 8555 | FAX +66 0 3304 8556
ALS LABORATORY GROUP (THAILAND) CO., LTD. An ALS Limited Company

Life Sciences

www.alsglobal.com

RIGHT SOLUTIONS RIGHT PARTNER



Analysis / Test Report

TESTING
No.0042

Client : Dow Chemical Thailand Ltd.

10 Moo 2, Asia Industrial Estate, Tambol Banchang, Amphur Banchang, Rayong Thailand 21130

P/O : 4516938776

Project Name : Environmental Quality Monitoring

Project Location : AIE_PG Plant

Lot ID: 2518560

Date Received : May 06, 2025

Date Reported : May 13, 2025

Report Number: 3303642-1

Page 1 of 1

Sample Number 2518560-4
Parameter Noise (Leq 24 hrs.)
Location กลุ่มบ้านประทุมมิตร (ที่อยู่ใกล้พื้นที่โครงการมากที่สุด) (GPS 47P 0726338, 1405748)
Measurement Date May 01 - May 02, 2025
Measurement by Sitpawit Suwannarat
Sound Level meter Serial No. 1173610

Time	Leq (dB(A))	Lmax (dB(A))	L90 (dB(A))
11:00 AM - 12:00 PM	53.8	81.8	44.3
12:00 PM - 01:00 PM	53.3	77.6	43.1
01:00 PM - 02:00 PM	52.4	76.7	45.5
02:00 PM - 03:00 PM	52.7	70.4	45.5
03:00 PM - 04:00 PM	52.1	77.2	44.9
04:00 PM - 05:00 PM	59.5	78.7	50.6
05:00 PM - 06:00 PM	51.7	74.6	41.4
06:00 PM - 07:00 PM	51.9	72.5	42.7
07:00 PM - 08:00 PM	50.4	74.4	44.8
08:00 PM - 09:00 PM	49.3	76.1	44.6
09:00 PM - 10:00 PM	47.3	68.0	44.5
10:00 PM - 11:00 PM	62.5	85.7	46.7
11:00 PM - 12:00 AM	49.0	69.7	47.6
12:00 AM - 01:00 AM	57.8	85.2	47.5
01:00 AM - 02:00 AM	48.1	63.7	46.7
02:00 AM - 03:00 AM	44.5	73.0	42.9
03:00 AM - 04:00 AM	45.1	75.5	42.2
04:00 AM - 05:00 AM	46.8	61.9	44.4
05:00 AM - 06:00 AM	50.7	67.8	45.0
06:00 AM - 07:00 AM	55.8	84.0	45.1
07:00 AM - 08:00 AM	54.8	76.5	44.5
08:00 AM - 09:00 AM	51.0	75.8	41.8
09:00 AM - 10:00 AM	63.3	89.4	42.8
10:00 AM - 11:00 AM	56.2	87.0	45.2

Leq Average 24 hrs. (dB(A)) 55.5
Lmax (dB(A)) 89.4
L90 (dB(A)) 44.6
Ldn (dB(A)) 61.8
Standard (dB(A)) 70 115

Reference Method : ISO1996-1 and 1996-2

Standard : 1. ประกาศคณะกรรมการสิ่งแวดล้อมแห่งชาติ ฉบับที่ 15 (พ.ศ. 2540) เรื่องกำหนดมาตรฐานระดับเสียงโดยทั่วไป
2. ประกาศกระทรวงอุตสาหกรรม เรื่องกำหนดค่าระดับเสียงการรบกวน และระดับเสียงที่เกิดจากการประกอบกิจการโรงงาน พ.ศ. 2548

Remark : The laboratory has been accepted as an accredited laboratory complying with the ISO/IEC 17025.

Technical Management

Chontichak

Chonticha Subongkoch
Scientist (3)

Approved by

Supot S

Supot Salamteh
Section Head

ADDRESS 616/10 Moo 5 T. Maenam Khu A. Pluakdaeng Rayong 21140 Thailand | PHONE +66 0 3304 8555 | FAX +66 0 3304 8556
ALS LABORATORY GROUP (THAILAND) CO., LTD. An ALS Limited Company

Life Sciences

www.alsglobal.com

RIGHT SOLUTIONS RIGHT PARTNER



Analysis / Test Report

TESTING
No.0042

Client : Dow Chemical Thailand Ltd.

10 Moo 2, Asia Industrial Estate, Tambol Banchang, Amphur Banchang, Rayong Thailand 21130

P/O : 4516938776

Project Name : Environmental Quality Monitoring

Project Location : AIE_PG Plant

Lot ID: 2518560

Date Received : May 06, 2025

Date Reported : May 13, 2025

Report Number: 3303643-1

Page 1 of 1

Sample Number 2518560-5
Parameter Noise (Leq 24 hrs.)
Location กลุ่มบ้านประทุมมิตร (ที่อยู่ใกล้พื้นที่โครงการมากที่สุด) (GPS 47P 0726338, 1405748)
Measurement Date May 02 - May 03, 2025
Measurement by Sitpawit Suwannarat
Sound Level meter Serial No. 1173610

Time	Leq (dB(A))	Lmax (dB(A))	L90 (dB(A))
11:00 AM - 12:00 PM	50.3	73.0	43.0
12:00 PM - 01:00 PM	48.2	67.3	39.6
01:00 PM - 02:00 PM	50.8	79.3	40.0
02:00 PM - 03:00 PM	54.9	82.6	40.2
03:00 PM - 04:00 PM	57.0	85.3	41.7
04:00 PM - 05:00 PM	52.5	84.3	43.6
05:00 PM - 06:00 PM	51.7	74.7	45.0
06:00 PM - 07:00 PM	54.9	81.3	45.2
07:00 PM - 08:00 PM	50.4	65.9	47.8
08:00 PM - 09:00 PM	50.6	71.0	46.7
09:00 PM - 10:00 PM	53.9	81.9	46.1
10:00 PM - 11:00 PM	46.0	60.4	43.6
11:00 PM - 12:00 AM	44.3	58.1	42.8
12:00 AM - 01:00 AM	45.1	62.7	43.3
01:00 AM - 02:00 AM	47.3	72.3	43.9
02:00 AM - 03:00 AM	53.1	77.2	44.6
03:00 AM - 04:00 AM	59.5	81.1	58.1
04:00 AM - 05:00 AM	60.4	84.1	59.0
05:00 AM - 06:00 AM	58.4	78.3	56.7
06:00 AM - 07:00 AM	58.6	88.1	51.8
07:00 AM - 08:00 AM	55.6	72.7	51.9
08:00 AM - 09:00 AM	54.9	81.3	46.8
09:00 AM - 10:00 AM	55.5	83.8	42.4
10:00 AM - 11:00 AM	52.2	78.3	42.2

Leq Average 24 hrs. (dB(A)) 54.7
Lmax (dB(A)) 88.1
L90 (dB(A)) 43.9
Ldn (dB(A)) 62.3
Standard (dB(A)) 70 115

Reference Method : ISO1996-1 and 1996-2

Standard : 1. ประกาศคณะกรรมการสิ่งแวดล้อมแห่งชาติ ฉบับที่ 15 (พ.ศ. 2540) เรื่องกำหนดมาตรฐานระดับเสียงโดยทั่วไป
2. ประกาศกระทรวงอุตสาหกรรม เรื่องกำหนดค่าระดับเสียงการรบกวน และระดับเสียงที่เกิดจากการประกอบกิจการโรงงาน พ.ศ. 2548

Remark : The laboratory has been accepted as an accredited laboratory complying with the ISO/IEC 17025.

Technical Management

Chontichak

Chonticha Subongkoch
Scientist (3)

Approved by

Supot S

Supot Salamteh
Section Head

ADDRESS 616/10 Moo 5 T. Maenam Khu A. Pluakdaeng Rayong 21140 Thailand | PHONE +66 0 3304 8555 | FAX +66 0 3304 8556
ALS LABORATORY GROUP (THAILAND) CO., LTD. An ALS Limited Company

Life Sciences

www.alsglobal.com

RIGHT SOLUTIONS RIGHT PARTNER



Analysis / Test Report

TESTING
No.0042

Client : Dow Chemical Thailand Ltd.

10 Moo 2, Asia Industrial Estate, Tambol Banchang, Amphur Banchang, Rayong Thailand 21130

P/O : 4516938776

Project Name : Environmental Quality Monitoring

Project Location : AIE_PG Plant

Lot ID: 2518560

Date Received : May 06, 2025

Date Reported : May 13, 2025

Report Number: 3303644-1

Page 1 of 1

Sample Number 2518560-6
Parameter Noise (Leq 24 hrs.)
Location กลุ่มบ้านประทุมมิตร (ที่อยู่ใกล้พื้นที่โครงการมากที่สุด) (GPS 47P 0726338, 1405748)
Measurement Date May 03 - May 04, 2025
Measurement by Sitpawit Suwannarat
Sound Level meter Serial No. 1173610

Time	Leq (dB(A))	Lmax (dB(A))	L90 (dB(A))
11:00 AM - 12:00 PM	52.4	74.8	44.4
12:00 PM - 01:00 PM	50.9	76.3	42.5
01:00 PM - 02:00 PM	50.9	75.4	41.3
02:00 PM - 03:00 PM	51.2	83.1	40.6
03:00 PM - 04:00 PM	51.3	70.1	44.0
04:00 PM - 05:00 PM	51.9	82.5	47.8
05:00 PM - 06:00 PM	55.9	87.3	48.0
06:00 PM - 07:00 PM	55.7	80.6	49.0
07:00 PM - 08:00 PM	56.1	75.6	51.0
08:00 PM - 09:00 PM	53.1	70.2	51.3
09:00 PM - 10:00 PM	53.7	65.4	52.9
10:00 PM - 11:00 PM	53.4	68.1	52.6
11:00 PM - 12:00 AM	52.8	72.4	51.5
12:00 AM - 01:00 AM	51.3	63.5	50.5
01:00 AM - 02:00 AM	50.8	58.7	49.8
02:00 AM - 03:00 AM	51.7	58.8	50.8
03:00 AM - 04:00 AM	52.0	69.0	51.0
04:00 AM - 05:00 AM	52.3	72.6	50.3
05:00 AM - 06:00 AM	52.8	81.5	47.0
06:00 AM - 07:00 AM	52.1	76.8	43.4
07:00 AM - 08:00 AM	57.0	78.0	46.2
08:00 AM - 09:00 AM	52.5	81.8	44.1
09:00 AM - 10:00 AM	57.4	92.7	42.4
10:00 AM - 11:00 AM	53.9	82.0	40.6

Leq Average 24 hrs. (dB(A)) 53.5
Lmax (dB(A)) 92.7
L90 (dB(A)) 47.8
Ldn (dB(A)) 59.0
Standard (dB(A)) 70 115

Reference Method : ISO1996-1 and 1996-2

Standard : 1. ประกาศคณะกรรมการสิ่งแวดล้อมแห่งชาติ ฉบับที่ 15 (พ.ศ. 2540) เรื่องกำหนดมาตรฐานระดับเสียงโดยทั่วไป
2. ประกาศกระทรวงอุตสาหกรรม เรื่องกำหนดค่าระดับเสียงการรบกวน และระดับเสียงที่เกิดจากการประกอบกิจการโรงงาน พ.ศ. 2548

Remark : The laboratory has been accepted as an accredited laboratory complying with the ISO/IEC 17025.

Technical Management

Chontichak

Chonticha Subongkoch
Scientist (3)

Approved by

Supot S

Supot Salamteh
Section Head

ADDRESS 616/10 Moo 5 T. Maenam Khu A. Pluakdaeng Rayong 21140 Thailand | PHONE +66 0 3304 8555 | FAX +66 0 3304 8556
ALS LABORATORY GROUP (THAILAND) CO., LTD. An ALS Limited Company

Life Sciences

www.alsglobal.com

RIGHT SOLUTIONS RIGHT PARTNER



Analysis / Test Report

TESTING
No.0042

Client : Dow Chemical Thailand Ltd.

10 Moo 2, Asia Industrial Estate, Tambol Banchang, Amphur Banchang, Rayong Thailand 21130

P/O : 4516938776

Project Name : Environmental Quality Monitoring

Project Location : AIE_PG Plant

Lot ID: 2518560

Date Received : May 06, 2025

Date Reported : May 13, 2025

Report Number: 3303645-1

Page 1 of 1

Sample Number 2518560-7
Parameter Noise (Leq 24 hrs.)
Location กลุ่มบ้านประทุมมิตร (ที่อยู่ใกล้พื้นที่โครงการมากที่สุด) (GPS 47P 0726338, 1405748)
Measurement Date May 04 - May 05, 2025
Measurement by Sitpawit Suwannarat
Sound Level meter Serial No. 1173610

Time	Leq (dB(A))	Lmax (dB(A))	L90 (dB(A))
11:00 AM - 12:00 PM	51.3	74.9	40.4
12:00 PM - 01:00 PM	47.9	74.6	41.9
01:00 PM - 02:00 PM	47.8	73.2	42.5
02:00 PM - 03:00 PM	50.5	77.0	42.6
03:00 PM - 04:00 PM	47.7	71.0	42.2
04:00 PM - 05:00 PM	50.6	76.6	43.2
05:00 PM - 06:00 PM	53.6	83.8	43.6
06:00 PM - 07:00 PM	54.0	82.1	45.1
07:00 PM - 08:00 PM	55.8	82.8	49.5
08:00 PM - 09:00 PM	50.5	62.5	48.7
09:00 PM - 10:00 PM	51.2	61.6	49.9
10:00 PM - 11:00 PM	52.7	79.7	50.1
11:00 PM - 12:00 AM	53.0	77.1	49.7
12:00 AM - 01:00 AM	49.4	64.1	48.1
01:00 AM - 02:00 AM	49.0	66.8	47.3
02:00 AM - 03:00 AM	48.6	57.6	47.2
03:00 AM - 04:00 AM	47.8	58.6	46.6
04:00 AM - 05:00 AM	48.3	63.4	46.4
05:00 AM - 06:00 AM	51.4	71.3	47.3
06:00 AM - 07:00 AM	55.9	86.4	44.6
07:00 AM - 08:00 AM	52.9	77.0	44.4
08:00 AM - 09:00 AM	51.6	75.9	44.0
09:00 AM - 10:00 AM	50.6	59.6	49.2
10:00 AM - 11:00 AM	49.8	60.6	48.6

Leq Average 24 hrs. (dB(A)) 51.6
Lmax (dB(A)) 86.4
L90 (dB(A)) 46.4
Ldn (dB(A)) 58.0
Standard (dB(A)) 70 115

Reference Method : ISO1996-1 and 1996-2

Standard : 1. ประกาศคณะกรรมการสิ่งแวดล้อมแห่งชาติ ฉบับที่ 15 (พ.ศ. 2540) เรื่องกำหนดมาตรฐานระดับเสียงโดยทั่วไป
2. ประกาศกระทรวงอุตสาหกรรม เรื่องกำหนดค่าระดับเสียงการรบกวน และระดับเสียงที่เกิดจากการประกอบกิจการโรงงาน พ.ศ. 2548

Remark : The laboratory has been accepted as an accredited laboratory complying with the ISO/IEC 17025.

Technical Management

Chontichak

Chonticha Subongkoch
Scientist (3)

Approved by

Supot S

Supot Salamteh
Section Head

ADDRESS 616/10 Moo 5 T. Maenam Khu A. Pluakdaeng Rayong 21140 Thailand | PHONE +66 0 3304 8555 | FAX +66 0 3304 8556
ALS LABORATORY GROUP (THAILAND) CO., LTD. An ALS Limited Company

Life Sciences

www.alsglobal.com

RIGHT SOLUTIONS RIGHT PARTNER



Analysis / Test Report

TESTING
No.0042

Client : Dow Chemical Thailand Ltd.

10 Moo 2, Asia Industrial Estate, Tambol Banchang, Amphur Banchang, Rayong Thailand 21130

P/O : 4516938776

Project Name : Environmental Quality Monitoring

Project Location : AIE_PG Plant

Lot ID: 2518560

Date Received : May 06, 2025

Date Reported : May 13, 2025

Report Number: 3303646-1

Page 1 of 1

Sample Number	2518560-8
Parameter	Noise (Leq 24 hrs.)
Location	กลุ่มบ้านปูนปนร ชย 17 ' พะนาลรัณนี ' ๓ พากาไมกั "ดัว) (GPS 47P 0727177, 1404390)
Measurement Date	Apr 28 - Apr 29, 2025
Measurement by	Sitpawit Suwannarat
Sound Level meter	Serial No. 1173609

Time	Leq (dB(A))	Lmax (dB(A))	L90 (dB(A))
10:00 AM - 11:00 AM	52.7	83.4	45.4
11:00 AM - 12:00 PM	52.5	82.2	45.9
12:00 PM - 01:00 PM	55.3	82.1	45.9
01:00 PM - 02:00 PM	49.9	70.8	46.6
02:00 PM - 03:00 PM	55.9	82.6	47.3
03:00 PM - 04:00 PM	56.5	82.7	47.1
04:00 PM - 05:00 PM	51.8	80.7	47.0
05:00 PM - 06:00 PM	55.9	81.6	47.2
06:00 PM - 07:00 PM	53.5	81.0	47.5
07:00 PM - 08:00 PM	55.1	83.3	48.5
08:00 PM - 09:00 PM	54.8	87.7	48.4
09:00 PM - 10:00 PM	56.1	85.2	48.9
10:00 PM - 11:00 PM	56.5	81.2	50.0
11:00 PM - 12:00 AM	55.9	71.8	51.2
12:00 AM - 01:00 AM	54.5	76.5	51.4
01:00 AM - 02:00 AM	52.7	66.0	50.9
02:00 AM - 03:00 AM	53.6	66.7	51.4
03:00 AM - 04:00 AM	54.9	74.2	51.4
04:00 AM - 05:00 AM	60.7	86.2	54.0
05:00 AM - 06:00 AM	57.8	73.3	53.7
06:00 AM - 07:00 AM	58.1	74.6	51.4
07:00 AM - 08:00 AM	64.4	79.2	51.4
08:00 AM - 09:00 AM	65.2	80.4	50.6
09:00 AM - 10:00 AM	66.3	82.4	50.7
Leq Average 24 hrs. (dB(A))	58.8		
Lmax (dB(A))		87.7	
L90 (dB(A))			48.9
Ldn (dB(A))	63.7		
Standard (dB(A))	70	115	
Reference Method : ISO1996-1 and 1996-2			
Standard : 1. คิงกาสุ ดงกไมกาใน 'พอนโล้งนถว'ปาฬคณบิ '๗5 (ร .ส. 2540) ใช้ท้าวานโมมาทฐานใจโรบิ ตพโยโธ 'นโค			
2. คิงกาสกจิ ในเพทหิ ววกไมใช้ท้าวานรู '่าใจโรบิ ตพทาใวมกเน ถลงใจโรบิ ตพิ 'ตติจจากกาไคจกทชภศกาใ			
ยไฟทจน ร .ส. 2548			
Remark : The laboratory has been accepted as an accredited laboratory complying with the ISO/IEC 17025.			

Technical Management

Chontichak.

Chonticha Subongkoch
Scientist (3)

Approved by

Snyp S.

Supot Salamteh
Section Head

ADDRESS 616/10 Moo 5 T. Maenam Khu A. Pluakdaeng Rayong 21140 Thailand | PHONE +66 0 3304 8555 | FAX +66 0 3304 8556
ALS LABORATORY GROUP (THAILAND) CO., LTD. An ALS Limited Company

Life Sciences

www.alsglobal.com

RIGHT SOLUTIONS RIGHT PARTNER



TESTING
No.0042

Lot ID: 2518560

Date Received : May 06, 2025

Date Reported : May 13, 2025

Report Number: 3303647-1

Page 1 of 1

Technical Management

Chonticha Subongkoch
Scientist (3)

Approved by

Supot Salamteh
Section Head

Life Sciences

www.alsglobal.com

RIGHT SOLUTIONS RIGHT PARTNER



Analysis / Test Report

TESTING
No.0042

Client : Dow Chemical Thailand Ltd.

10 Moo 2, Asia Industrial Estate, Tambol Banchang, Amphur Banchang, Rayong Thailand 21130

P/O : 4516938776

Project Name : Environmental Quality Monitoring

Project Location : AIE_PG Plant

Lot ID: 2518560

Date Received : May 06, 2025

Date Reported : May 13, 2025

Report Number: 3303648-1

Page 1 of 1

Sample Number	2518560-10
Parameter	Noise (Leq 24 hrs.)
Location	กลุ่มบ้านปูนปนร ชย 17 (ต. ชัยนาท น. 17) ใกล้วัดบ้านใหม่ (วัดใหม่) (GPS 47P 0727177, 1404390)
Measurement Date	Apr 30 - May 01, 2025
Measurement by	Sitpawit Suwannarat
Sound Level meter	Serial No. 1173609

Time	Leq (dB(A))	Lmax (dB(A))	L90 (dB(A))
10:00 AM - 11:00 AM	55.2	82.3	46.7
11:00 AM - 12:00 PM	55.9	87.0	46.3
12:00 PM - 01:00 PM	50.5	70.8	46.3
01:00 PM - 02:00 PM	54.6	80.0	47.3
02:00 PM - 03:00 PM	55.1	79.9	48.3
03:00 PM - 04:00 PM	55.2	81.0	49.0
04:00 PM - 05:00 PM	54.1	82.2	48.2
05:00 PM - 06:00 PM	54.9	87.5	47.4
06:00 PM - 07:00 PM	54.1	71.2	47.3
07:00 PM - 08:00 PM	49.6	63.6	48.4
08:00 PM - 09:00 PM	49.2	66.6	47.4
09:00 PM - 10:00 PM	62.8	88.8	47.6
10:00 PM - 11:00 PM	53.3	81.3	48.4
11:00 PM - 12:00 AM	56.6	73.5	48.9
12:00 AM - 01:00 AM	58.9	75.6	50.1
01:00 AM - 02:00 AM	58.9	77.1	48.6
02:00 AM - 03:00 AM	69.3	78.3	48.8
03:00 AM - 04:00 AM	67.9	81.1	50.9
04:00 AM - 05:00 AM	60.6	82.5	51.5
05:00 AM - 06:00 AM	60.4	87.5	52.3
06:00 AM - 07:00 AM	59.2	82.5	52.4
07:00 AM - 08:00 AM	58.5	83.3	49.2
08:00 AM - 09:00 AM	52.0	82.1	46.1
09:00 AM - 10:00 AM	54.4	81.1	45.8
Leq Average 24 hrs. (dB(A))	60.3		
Lmax (dB(A))		88.8	
L90 (dB(A))			48.3
Ldn (dB(A))	69.3		
Standard (dB(A))	70	115	
Reference Method : ISO1996-1 and 1996-2			
Standard : 1. ค.ในกาส ดงกไมกาน 'คณโลจันถว'ปาหคณบิ 'ศ5 (ร.ส. 2540) ใชหทวานโมหาฐานในวิบิ ตพยโร 'นโค			
2. ค.ในกาสกจิ ในเขตหิ ววกไม ใชหทวาน 'าในวิบิ ตพทาในกณ ถลงในวิบิ ตพ 'ตติจากกาไคในกททกศกาใ			
ยไฟทน ร.ส. 2548			
Remark : The laboratory has been accepted as an accredited laboratory complying with the ISO/IEC 17025.			

Technical Management

Chontichak.

Chonticha Subongkoch
Scientist (3)

Approved by

Snyp S.

Supot Salamteh
Section Head

ADDRESS 616/10 Moo 5 T. Maenam Khu A. Pluakdaeng Rayong 21140 Thailand | PHONE +66 0 3304 8555 | FAX +66 0 3304 8556
ALS LABORATORY GROUP (THAILAND) CO., LTD. An ALS Limited Company

Life Sciences

www.alsglobal.com

RIGHT SOLUTIONS RIGHT PARTNER



Analysis / Test Report

TESTING
No.0042

Client : Dow Chemical Thailand Ltd.

10 Moo 2, Asia Industrial Estate, Tambol Banchang, Amphur Banchang, Rayong Thailand 21130

P/O : 4516938776

Project Name : Environmental Quality Monitoring

Project Location : AIE_PG Plant

Lot ID: 2518560

Date Received : May 06, 2025

Date Reported : May 13, 2025

Report Number: 3303649-1

Page 1 of 1

Sample Number	2518560-11
Parameter	Noise (Leq 24 hrs.)
Location	กลุ่มบ้านปูนปนร ชย 17 (ซอยบางลำภวนี ๓ พหลโยธิน) (GPS 47P 0727177, 1404390)
Measurement Date	May 01 - May 02, 2025
Measurement by	Sitpawit Suwannarat
Sound Level meter	Serial No. 1173609

Time	Leq (dB(A))	Lmax (dB(A))	L90 (dB(A))
10:00 AM - 11:00 AM	55.0	81.2	45.6
11:00 AM - 12:00 PM	50.3	79.2	45.5
12:00 PM - 01:00 PM	54.4	80.1	45.7
01:00 PM - 02:00 PM	52.0	79.5	46.0
02:00 PM - 03:00 PM	53.6	81.8	47.0
03:00 PM - 04:00 PM	53.3	86.2	46.9
04:00 PM - 05:00 PM	54.6	83.7	47.4
05:00 PM - 06:00 PM	55.0	79.7	48.5
06:00 PM - 07:00 PM	54.4	70.3	49.7
07:00 PM - 08:00 PM	53.0	75.0	49.9
08:00 PM - 09:00 PM	51.2	64.5	49.4
09:00 PM - 10:00 PM	52.1	65.2	49.9
10:00 PM - 11:00 PM	53.4	72.7	49.9
11:00 PM - 12:00 AM	59.2	84.7	52.5
12:00 AM - 01:00 AM	56.3	71.8	52.2
01:00 AM - 02:00 AM	56.6	73.1	49.9
02:00 AM - 03:00 AM	62.9	77.7	49.9
03:00 AM - 04:00 AM	63.7	78.9	49.1
04:00 AM - 05:00 AM	64.8	80.9	49.2
05:00 AM - 06:00 AM	57.1	84.3	50.9
06:00 AM - 07:00 AM	56.1	82.4	48.2
07:00 AM - 08:00 AM	54.2	80.2	46.2
08:00 AM - 09:00 AM	55.5	81.5	46.1
09:00 AM - 10:00 AM	53.2	80.5	46.1
Leq Average 24 hrs. (dB(A))	57.6		
Lmax (dB(A))		86.2	
L90 (dB(A))			48.5
Ldn (dB(A))	66.4		
Standard (dB(A))	70	115	
Reference Method : ISO1996-1 and 1996-2			
Standard : 1. คิงกาส ดงกไมกาโ คนโล้นถวปาหคณบี ๗5 (ร.ส. 2540) โะเพทวอนโมหาไลรานงอโน โทยโอ นโค			
2. คิงกาสกจิ ในเทหาววกไม โะเพทวอนเ วาองโน โทะพาโในกน ถลงงอโน โทฟ โทะจิกากาโคงกขบคศกาไ			
ยโพทน ร .ส. 2548			
Remark : The laboratory has been accepted as an accredited laboratory complying with the ISO/IEC 17025.			

Technical Management

Chontichak

Chonticha Subongkoch
Scientist (3)

Approved by

Snapt S.

Supot Salamteh
Section Head

ADDRESS 616/10 Moo 5 T. Maenam Khu A. Pluakdaeng Rayong 21140 Thailand | PHONE +66 0 3304 8555 | FAX +66 0 3304 8556
ALS LABORATORY GROUP (THAILAND) CO., LTD. An ALS Limited Company

Life Sciences

www.alsglobal.com

RIGHT SOLUTIONS RIGHT PARTNER



Analysis / Test Report

TESTING
No.0042

Client : Dow Chemical Thailand Ltd.
10 Moo 2, Asia Industrial Estate, Tambol Banchang, Amphur Banchang, Rayong Thailand 21130
P/O : 4516938776
Project Name : Environmental Quality Monitoring
Project Location : AIE_PG Plant

Lot ID: 2518560

Date Received : May 06, 2025
Date Reported : May 13, 2025
Report Number: 3303650-1

Page 1 of 1

Sample Number 2518560-12
Parameter Noise (Leq 24 hrs.)
Location กลุ่มบ้านปูนปนร ะ 1 (ซ. ชลบุรี 111) ใกล้วัดบ้านใหม่ (GPS 47P 0727177, 1404390)
Measurement Date May 02 - May 03, 2025
Measurement by Sitpawit Suwannarat
Sound Level meter Serial No. 1173609

Time	Leq (dB(A))	Lmax (dB(A))	L90 (dB(A))
10:00 AM - 11:00 AM	52.1	81.7	46.3
11:00 AM - 12:00 PM	53.6	79.9	46.2
12:00 PM - 01:00 PM	48.7	69.4	46.1
01:00 PM - 02:00 PM	53.8	80.5	46.4
02:00 PM - 03:00 PM	55.7	83.0	46.7
03:00 PM - 04:00 PM	50.3	72.0	46.6
04:00 PM - 05:00 PM	55.3	81.7	46.9
05:00 PM - 06:00 PM	52.8	73.3	46.8
06:00 PM - 07:00 PM	55.0	74.6	48.5
07:00 PM - 08:00 PM	53.5	60.0	49.6
08:00 PM - 09:00 PM	54.0	60.2	51.3
09:00 PM - 10:00 PM	53.1	67.3	50.5
10:00 PM - 11:00 PM	51.6	62.9	47.8
11:00 PM - 12:00 AM	52.1	66.0	48.3
12:00 AM - 01:00 AM	50.9	76.3	47.0
01:00 AM - 02:00 AM	69.2	104.7	42.4
02:00 AM - 03:00 AM	64.7	90.0	53.5
03:00 AM - 04:00 AM	61.1	82.6	52.7
04:00 AM - 05:00 AM	69.9	84.0	53.6
05:00 AM - 06:00 AM	60.1	84.0	50.5
06:00 AM - 07:00 AM	55.8	81.7	50.1
07:00 AM - 08:00 AM	52.8	70.8	48.4
08:00 AM - 09:00 AM	58.4	84.3	47.1
09:00 AM - 10:00 AM	52.0	74.0	45.7

Leq Average 24 hrs. (dB(A)) 60.7
Lmax (dB(A)) 104.7
L90 (dB(A)) 47.1
Ldn (dB(A)) 70.1
Standard (dB(A)) 70 115

Reference Method : ISO1996-1 and 1996-2

Standard : 1. คิงกาสุ ดงกโมก้า โชนโลล์ทอว่ฟลาคอบบิ ๗5 (ร.ส. 2540) เข็ททว่นโมหไธว่นไงไบไ ๗เพไะ ๗ไค
2. คิงกาสุกจิ ในททท ๗วกโม เข็ททว่น ๗ไงไบไ ๗ททวโมกณ ถลนไงไบไ ๗พิ ๗ไคจากกาไคไงททททททไ
๗ไฟททท ร.ส. 2548

Remark : The laboratory has been accepted as an accredited laboratory complying with the ISO/IEC 17025.

Technical Management

Chontichak

Chonticha Subongkoch
Scientist (3)

Approved by

Supot S

Supot Salamteh
Section Head

ADDRESS 616/10 Moo 5 T. Maenam Khu A. Pluakdaeng Rayong 21140 Thailand | PHONE +66 0 3304 8555 | FAX +66 0 3304 8556
ALS LABORATORY GROUP (THAILAND) CO., LTD. An ALS Limited Company

Life Sciences

www.alsglobal.com

RIGHT SOLUTIONS RIGHT PARTNER



Analysis / Test Report

TESTING
No.0042

Client : Dow Chemical Thailand Ltd.

10 Moo 2, Asia Industrial Estate, Tambol Banchang, Amphur Banchang, Rayong Thailand 21130

P/O : 4516938776

Project Name : Environmental Quality Monitoring

Project Location : AIE_PG Plant

Lot ID: 2518560

Date Received : May 06, 2025

Date Reported : May 13, 2025

Report Number: 3303651-1

Page 1 of 1

Sample Number 2518560-13
Parameter Noise (Leq 24 hrs.)
Location กลุ่มบ้านปูนปนระ ๑ (ซ. ชลบุรี ๑๑๑) (GPS 47P 0727177, 1404390)
Measurement Date May 03 - May 04, 2025
Measurement by Sitpawit Suwannarat
Sound Level meter Serial No. 1173609

Time	Leq (dB(A))	Lmax (dB(A))	L90 (dB(A))
10:00 AM - 11:00 AM	55.6	80.8	45.8
11:00 AM - 12:00 PM	55.1	81.8	45.6
12:00 PM - 01:00 PM	59.1	82.3	46.8
01:00 PM - 02:00 PM	66.1	87.5	46.5
02:00 PM - 03:00 PM	61.3	87.2	49.2
03:00 PM - 04:00 PM	56.1	81.3	52.7
04:00 PM - 05:00 PM	53.9	72.4	52.1
05:00 PM - 06:00 PM	56.0	71.7	53.2
06:00 PM - 07:00 PM	57.9	69.3	54.0
07:00 PM - 08:00 PM	54.2	65.0	50.8
08:00 PM - 09:00 PM	51.7	62.0	49.7
09:00 PM - 10:00 PM	54.6	71.5	50.6
10:00 PM - 11:00 PM	57.5	72.5	49.9
11:00 PM - 12:00 AM	61.2	86.1	49.3
12:00 AM - 01:00 AM	56.9	74.3	51.1
01:00 AM - 02:00 AM	59.7	75.0	52.3
02:00 AM - 03:00 AM	68.2	78.6	52.3
03:00 AM - 04:00 AM	69.4	78.0	65.6
04:00 AM - 05:00 AM	66.9	76.7	48.5
05:00 AM - 06:00 AM	64.9	95.0	49.0
06:00 AM - 07:00 AM	65.7	91.6	55.0
07:00 AM - 08:00 AM	57.1	91.2	51.4
08:00 AM - 09:00 AM	59.6	84.2	49.8
09:00 AM - 10:00 AM	56.9	82.1	48.5

Leq Average 24 hrs. (dB(A)) 62.4
Lmax (dB(A)) 95.0
L90 (dB(A)) 49.9
Ldn (dB(A)) 71.2
Standard (dB(A)) 70 115

Reference Method : ISO1996-1 and 1996-2

Standard : 1. คิงกาสุ ดงกโมก้า โชนโลลันถอ'พลาหคณบิ' ๗5 (ร.ส. 2540) เชนทอวณโมหาไรนังโงโงโง โทพโยโง'นไค
2. คิงกาสุกจิ ในทอหิ วอวกโม เชนทอวณ'โงโงโงโง โทพโยโง'นไค โทพโยโง'นไค โทพโยโง'นไค โทพโยโง'นไค
ยโพทณ ร.ส. 2548

Remark : The laboratory has been accepted as an accredited laboratory complying with the ISO/IEC 17025.

Technical Management

Chontichak

Chonticha Subongkoch
Scientist (3)

Approved by

Supot S

Supot Salamteh
Section Head

ADDRESS 616/10 Moo 5 T. Maenam Khu A. Pluakdaeng Rayong 21140 Thailand | PHONE +66 0 3304 8555 | FAX +66 0 3304 8556
ALS LABORATORY GROUP (THAILAND) CO., LTD. An ALS Limited Company

Life Sciences

www.alsglobal.com

RIGHT SOLUTIONS RIGHT PARTNER



Analysis / Test Report

TESTING
No.0042

Client : Dow Chemical Thailand Ltd.

10 Moo 2, Asia Industrial Estate, Tambol Banchang, Amphur Banchang, Rayong Thailand 21130

P/O : 4516938776

Project Name : Environmental Quality Monitoring

Project Location : AIE_PG Plant

Lot ID: 2518560

Date Received : May 06, 2025

Date Reported : May 13, 2025

Report Number: 3303652-1

Page 1 of 1

Sample Number 2518560-14
Parameter Noise (Leq 24 hrs.)
Location กลุ่มบ้านปูนปนร ะ 1 (ซ. ชลบุรี 111) ใกล้วัดบ้านใหม่ (GPS 47P 0727177, 1404390)
Measurement Date May 04 - May 05, 2025
Measurement by Sitpawit Suwannarat
Sound Level meter Serial No. 1173609

Time	Leq (dB(A))	Lmax (dB(A))	L90 (dB(A))
10:00 AM - 11:00 AM	51.6	70.1	47.7
11:00 AM - 12:00 PM	51.7	81.9	46.0
12:00 PM - 01:00 PM	50.7	81.5	45.9
01:00 PM - 02:00 PM	47.9	71.5	46.0
02:00 PM - 03:00 PM	54.2	81.4	45.8
03:00 PM - 04:00 PM	55.1	80.8	46.3
04:00 PM - 05:00 PM	53.5	79.9	47.6
05:00 PM - 06:00 PM	54.8	81.2	48.2
06:00 PM - 07:00 PM	57.1	72.3	49.3
07:00 PM - 08:00 PM	55.9	76.4	50.8
08:00 PM - 09:00 PM	52.2	61.5	49.9
09:00 PM - 10:00 PM	55.5	70.7	50.1
10:00 PM - 11:00 PM	57.6	73.2	49.9
11:00 PM - 12:00 AM	54.8	72.0	51.5
12:00 AM - 01:00 AM	56.6	72.6	52.0
01:00 AM - 02:00 AM	68.9	77.0	50.3
02:00 AM - 03:00 AM	68.3	74.1	50.2
03:00 AM - 04:00 AM	69.0	77.2	65.4
04:00 AM - 05:00 AM	68.8	82.1	49.5
05:00 AM - 06:00 AM	57.7	82.5	49.5
06:00 AM - 07:00 AM	53.6	81.7	46.9
07:00 AM - 08:00 AM	54.6	80.9	45.7
08:00 AM - 09:00 AM	55.6	83.7	48.9
09:00 AM - 10:00 AM	56.6	82.9	47.7

Leq Average 24 hrs. (dB(A)) 61.8
Lmax (dB(A)) 83.7
L90 (dB(A)) 48.9
Ldn (dB(A)) 71.3
Standard (dB(A)) 70 115

Reference Method : ISO1996-1 and 1996-2

Standard : 1. คิงกาส ดงกโมก้า โชนโลชั่นมอ'พลาหคณบิ 5 (ร.ส. 2540) ใชท้าวานโมหาไรานใจโบเ ทยโย ันไค
2. คิงกาสกจิ ในทหิ ววกโม ใชท้าวาน ำใจโบเ ทยโยโมกณ ถลงใจโบเ ทย ติจจากกาไคใจททกททกา
ยโพทท ร.ส. 2548

Remark : The laboratory has been accepted as an accredited laboratory complying with the ISO/IEC 17025.

Technical Management

Chontichak

Chonticha Subongkoch
Scientist (3)

Approved by

Supot S

Supot Salamteh
Section Head

ADDRESS 616/10 Moo 5 T. Maenam Khu A. Pluakdaeng Rayong 21140 Thailand | PHONE +66 0 3304 8555 | FAX +66 0 3304 8556
ALS LABORATORY GROUP (THAILAND) CO., LTD. An ALS Limited Company

Life Sciences

www.alsglobal.com

RIGHT SOLUTIONS RIGHT PARTNER

ภาคผนวก ค-3

ผลการตรวจวัดระดับเสียงโดยทั่วไปบริเวณพื้นที่โครงการ



Analysis / Test Report

TESTING
No.0042

Client : Dow Chemical Thailand Ltd.
10 Moo 2, Asia Industrial Estate, Tambol Banchang, Amphur Banchang, Rayong Thailand 21130

P/O :

Project Name : Environmental Quality Monitoring

Project Location : AIE_PG Plant

Lot ID: 2518295

Date Received : May 06, 2025

Date Reported : May 20, 2025

Report Number: 3303693-1C16

Page 1 of 1

Sample Number 2518295-1
Parameter Noise (Leq 24 hrs.)
Location บริเวณริมรั้วของโครงการทางด้านทิศตะวันตกของพื้นที่ HPPO (GPS 47P 0726777, 1405417)
Measurement Date Apr 28 - Apr 29, 2025
Measurement by Sitpawit Suwannarat
Sound Level meter Serial No. 900071

Time	Leq (dB(A))	Lmax (dB(A))	L90 (dB(A))
12:00 PM - 01:00 PM	59.2	80.4	56.5
01:00 PM - 02:00 PM	58.3	70.5	56.7
02:00 PM - 03:00 PM	57.9	76.4	56.3
03:00 PM - 04:00 PM	60.6	88.8	56.4
04:00 PM - 05:00 PM	61.3	86.3	56.8
05:00 PM - 06:00 PM	59.1	80.1	56.6
06:00 PM - 07:00 PM	59.0	82.6	56.5
07:00 PM - 08:00 PM	58.2	73.9	56.9
08:00 PM - 09:00 PM	58.1	77.8	57.0
09:00 PM - 10:00 PM	58.1	68.0	57.5
10:00 PM - 11:00 PM	60.3	90.9	57.6
11:00 PM - 12:00 AM	57.8	66.7	57.2
12:00 AM - 01:00 AM	57.7	66.3	56.9
01:00 AM - 02:00 AM	57.4	66.3	56.9
02:00 AM - 03:00 AM	59.3	87.7	57.3
03:00 AM - 04:00 AM	57.0	67.5	55.6
04:00 AM - 05:00 AM	57.1	66.0	56.0
05:00 AM - 06:00 AM	57.8	76.3	55.8
06:00 AM - 07:00 AM	60.6	85.1	57.8
07:00 AM - 08:00 AM	62.1	87.6	57.2
08:00 AM - 09:00 AM	59.1	84.1	56.4
09:00 AM - 10:00 AM	58.6	81.8	56.2
10:00 AM - 11:00 AM	59.2	76.5	57.2
11:00 AM - 12:00 PM	58.0	75.7	55.7

Leq Average 24 hrs. (dB(A)) 59.0
Lmax (dB(A)) 90.9
L90 (dB(A)) 56.7
Ldn (dB(A)) 65.1
Standard (dB(A)) 70 115

Reference Method : ISO1996-1 and 1996-2

Standard : 1. ประกาศคณะกรรมการสิ่งแวดล้อมแห่งชาติ ฉบับที่ 15 (พ.ศ. 2540) เรื่องกำหนดมาตรฐานระดับเสียงโดยทั่วไป
2. ประกาศกระทรวงอุตสาหกรรม เรื่องกำหนดค่าระดับเสียงการรบกวน และระดับเสียงที่เกิดจากการประกอบกิจการโรงงาน พ.ศ. 2548

Technical Management

Chontichak

Chonticha Subongkoch
Scientist (3)

Approved by

Supot S

Supot Salamteh
Section Head

The above results are valid only for the analyzed/tested sample(s) as indicated in this report. No part of this report or certificate may be reproduced in any form without written consent from the Laboratory. ALS Laboratory Group (Thailand) strongly recommends that this report is not reproduced except in full.

ADDRESS 616/10 Moo 5 T. Maenam Khu A. Pluakdaeng Rayong 21140 Thailand | PHONE +66 0 3304 8555 | FAX +66 0 3304 8556

Life Sciences

www.alsglobal.com

RIGHT SOLUTIONS RIGHT PARTNER

8525-209/ EMAIL



Analysis / Test Report

TESTING
No.0042

Client : Dow Chemical Thailand Ltd.
10 Moo 2, Asia Industrial Estate, Tambol Banchang, Amphur Banchang, Rayong Thailand
21130

P/O :
Project Name : Environmental Quality Monitoring
Project Location : AIE_PG Plant

Lot ID: 2518295

Date Received : May 06, 2025
Date Reported : May 20, 2025
Report Number: 3303694-1C16

Page 1 of 1

Sample Number 2518295-2
Parameter Noise (Leq 24 hrs.)
Location บริเวณริมรั้วของโครงการทางด้านทิศตะวันตกของพื้นที่ HPPO (GPS 47P 0726777, 1405417)
Measurement Date Apr 29 - Apr 30, 2025
Measurement by Sitpawit Suwannarat
Sound Level meter Serial No. 900071

Time	Leq (dB(A))	Lmax (dB(A))	L90 (dB(A))
12:00 PM - 01:00 PM	58.0	75.1	55.4
01:00 PM - 02:00 PM	58.0	77.5	55.6
02:00 PM - 03:00 PM	59.8	85.2	56.9
03:00 PM - 04:00 PM	58.0	74.0	56.8
04:00 PM - 05:00 PM	62.6	94.6	56.7
05:00 PM - 06:00 PM	58.7	79.4	56.6
06:00 PM - 07:00 PM	59.9	80.7	56.8
07:00 PM - 08:00 PM	58.6	71.7	57.3
08:00 PM - 09:00 PM	58.9	78.7	57.8
09:00 PM - 10:00 PM	58.1	71.0	57.3
10:00 PM - 11:00 PM	58.1	80.6	57.3
11:00 PM - 12:00 AM	58.2	74.8	57.3
12:00 AM - 01:00 AM	57.7	69.5	57.1
01:00 AM - 02:00 AM	58.2	75.8	57.5
02:00 AM - 03:00 AM	58.4	81.9	57.5
03:00 AM - 04:00 AM	57.9	65.1	57.3
04:00 AM - 05:00 AM	58.1	66.7	57.5
05:00 AM - 06:00 AM	59.0	75.5	57.8
06:00 AM - 07:00 AM	60.5	83.9	57.9
07:00 AM - 08:00 AM	61.5	85.4	57.5
08:00 AM - 09:00 AM	58.9	79.4	56.3
09:00 AM - 10:00 AM	59.0	82.2	56.2
10:00 AM - 11:00 AM	57.6	77.0	56.0
11:00 AM - 12:00 PM	58.9	83.8	56.1

Leq Average 24 hrs. (dB(A)) 59.1
Lmax (dB(A)) 94.6
L90 (dB(A)) 57.1
Ldn (dB(A)) 65.1
Standard (dB(A)) 70 115

Reference Method : ISO1996-1 and 1996-2

Standard : 1. ประกาศคณะกรรมการสิ่งแวดล้อมแห่งชาติ ฉบับที่ 15 (พ.ศ. 2540) เรื่องกำหนดมาตรฐานระดับเสียงโดยทั่วไป
2. ประกาศกระทรวงอุตสาหกรรม เรื่องกำหนดค่าระดับเสียงการรบกวน และระดับเสียงที่เกิดจากการประกอบกิจการ
โรงงาน พ.ศ. 2548

Technical Management

Chontichak

Chonticha Subongkoch
Scientist (3)

Approved by

Supot S

Supot Salamteh
Section Head

The above results are valid only for the analyzed/tested sample(s) as indicated in this report. No part of this report or certificate may be reproduced in any form without written consent from the Laboratory. ALS Laboratory Group (Thailand) strongly recommends that this report is not reproduced except in full.

ADDRESS 616/10 Moo 5 T. Maenam Khu A. Pluakdaeng Rayong 21140 Thailand | PHONE +66 0 3304 8555 | FAX +66 0 3304 8556

Life Sciences

www.alsglobal.com

RIGHT SOLUTIONS RIGHT PARTNER

8525-209/ EMAIL



Analysis / Test Report

TESTING
No.0042

Client : Dow Chemical Thailand Ltd.
10 Moo 2, Asia Industrial Estate, Tambol Banchang, Amphur Banchang, Rayong Thailand
21130

P/O :

Project Name : Environmental Quality Monitoring

Project Location : AIE_PG Plant

Lot ID: 2518295

Date Received : May 06, 2025

Date Reported : May 20, 2025

Report Number: 3303695-1C16

Page 1 of 1

Sample Number 2518295-3
Parameter Noise (Leq 24 hrs.)
Location บริเวณริมรั้วของโครงการทางด้านทิศตะวันตกของพื้นที่ HPPO (GPS 47P 0726777, 1405417)
Measurement Date Apr 30 - May 01, 2025
Measurement by Sitpawit Suwannarat
Sound Level meter Serial No. 900071

Time	Leq (dB(A))	Lmax (dB(A))	L90 (dB(A))
12:00 PM - 01:00 PM	57.9	74.8	55.9
01:00 PM - 02:00 PM	58.3	78.7	56.0
02:00 PM - 03:00 PM	58.3	80.9	56.4
03:00 PM - 04:00 PM	57.6	78.3	55.9
04:00 PM - 05:00 PM	59.8	85.4	56.0
05:00 PM - 06:00 PM	58.7	77.5	56.1
06:00 PM - 07:00 PM	59.8	84.1	56.8
07:00 PM - 08:00 PM	58.5	72.8	56.9
08:00 PM - 09:00 PM	59.4	86.3	56.9
09:00 PM - 10:00 PM	58.5	78.8	57.3
10:00 PM - 11:00 PM	61.1	88.2	57.8
11:00 PM - 12:00 AM	59.7	70.1	58.8
12:00 AM - 01:00 AM	59.3	68.0	58.5
01:00 AM - 02:00 AM	58.6	69.0	58.0
02:00 AM - 03:00 AM	58.7	71.3	58.0
03:00 AM - 04:00 AM	59.2	63.2	58.7
04:00 AM - 05:00 AM	59.3	73.6	58.6
05:00 AM - 06:00 AM	58.7	72.0	57.7
06:00 AM - 07:00 AM	60.9	86.6	58.1
07:00 AM - 08:00 AM	60.0	84.9	56.9
08:00 AM - 09:00 AM	57.1	71.3	55.7
09:00 AM - 10:00 AM	56.8	71.6	55.5
10:00 AM - 11:00 AM	57.5	76.1	56.2
11:00 AM - 12:00 PM	59.6	86.7	56.3

Leq Average 24 hrs. (dB(A)) 59.0
Lmax (dB(A)) 88.2
L90 (dB(A)) 56.9
Ldn (dB(A)) 65.9
Standard (dB(A)) 70 115

Reference Method : ISO1996-1 and 1996-2

Standard : 1. ประกาศคณะกรรมการสิ่งแวดล้อมแห่งชาติ ฉบับที่ 15 (พ.ศ. 2540) เรื่องกำหนดมาตรฐานระดับเสียงโดยทั่วไป
2. ประกาศกระทรวงอุตสาหกรรม เรื่องกำหนดค่าระดับเสียงการรบกวน และระดับเสียงที่เกิดจากการประกอบกิจการ
โรงงาน พ.ศ. 2548

Technical Management

Chontichak

Chonticha Subongkoch
Scientist (3)

Approved by

Supot S

Supot Salamteh
Section Head

The above results are valid only for the analyzed/tested sample(s) as indicated in this report. No part of this report or certificate may be reproduced in any form without written consent from the Laboratory. ALS Laboratory Group (Thailand) strongly recommends that this report is not reproduced except in full.

ADDRESS 616/10 Moo 5 T. Maenam Khu A. Pluakdaeng Rayong 21140 Thailand | PHONE +66 0 3304 8555 | FAX +66 0 3304 8556

Life Sciences

www.alsglobal.com

RIGHT SOLUTIONS RIGHT PARTNER

8525-209/ EMAIL



Analysis / Test Report

TESTING
No.0042

Client : Dow Chemical Thailand Ltd.
10 Moo 2, Asia Industrial Estate, Tambol Banchang, Amphur Banchang, Rayong Thailand 21130

P/O :

Project Name : Environmental Quality Monitoring

Project Location : AIE_PG Plant

Lot ID: 2518295

Date Received : May 06, 2025

Date Reported : May 20, 2025

Report Number: 3303696-1C16

Page 1 of 1

Sample Number 2518295-4
Parameter Noise (Leq 24 hrs.)
Location บริเวณริมรั้วของโครงการทางด้านทิศตะวันตกของพื้นที่ HPPO (GPS 47P 0726777, 1405417)
Measurement Date May 01 - May 02, 2025
Measurement by Sitpawit Suwannarat
Sound Level meter Serial No. 900071

Time	Leq (dB(A))	Lmax (dB(A))	L90 (dB(A))
12:00 PM - 01:00 PM	57.4	72.4	55.8
01:00 PM - 02:00 PM	57.1	72.6	55.8
02:00 PM - 03:00 PM	56.4	71.4	54.7
03:00 PM - 04:00 PM	56.3	78.7	54.7
04:00 PM - 05:00 PM	57.0	76.6	55.0
05:00 PM - 06:00 PM	56.7	70.9	55.4
06:00 PM - 07:00 PM	58.1	79.8	56.0
07:00 PM - 08:00 PM	59.1	83.3	56.4
08:00 PM - 09:00 PM	58.1	70.9	57.1
09:00 PM - 10:00 PM	58.8	74.1	57.5
10:00 PM - 11:00 PM	58.6	71.9	57.7
11:00 PM - 12:00 AM	58.5	65.9	57.7
12:00 AM - 01:00 AM	59.0	79.7	57.8
01:00 AM - 02:00 AM	58.2	73.3	57.2
02:00 AM - 03:00 AM	57.6	67.6	56.8
03:00 AM - 04:00 AM	57.8	72.6	57.2
04:00 AM - 05:00 AM	58.1	67.2	57.4
05:00 AM - 06:00 AM	59.7	77.0	57.8
06:00 AM - 07:00 AM	61.6	83.0	57.7
07:00 AM - 08:00 AM	61.3	81.3	56.8
08:00 AM - 09:00 AM	59.1	79.3	56.2
09:00 AM - 10:00 AM	61.2	92.4	56.9
10:00 AM - 11:00 AM	59.0	74.8	57.3
11:00 AM - 12:00 PM	58.5	77.2	55.6

Leq Average 24 hrs. (dB(A)) 58.7
Lmax (dB(A)) 92.4
L90 (dB(A)) 56.8
Ldn (dB(A)) 65.3
Standard (dB(A)) 70 115

Reference Method : ISO1996-1 and 1996-2

Standard : 1. ประกาศคณะกรรมการสิ่งแวดล้อมแห่งชาติ ฉบับที่ 15 (พ.ศ. 2540) เรื่องกำหนดมาตรฐานระดับเสียงโดยทั่วไป
2. ประกาศกระทรวงอุตสาหกรรม เรื่องกำหนดค่าระดับเสียงการรบกวน และระดับเสียงที่เกิดจากการประกอบกิจการโรงงาน พ.ศ. 2548

Technical Management

Chontichak

Chonticha Subongkoch

Scientist (3)

Approved by

Supot S

Supot Salamteh

Section Head

The above results are valid only for the analyzed/tested sample(s) as indicated in this report. No part of this report or certificate may be reproduced in any form without written consent from the Laboratory. ALS Laboratory Group (Thailand) strongly recommends that this report is not reproduced except in full.

ADDRESS 616/10 Moo 5 T. Maenam Khu A. Pluakdaeng Rayong 21140 Thailand | PHONE +66 0 3304 8555 | FAX +66 0 3304 8556

Life Sciences

www.alsglobal.com

RIGHT SOLUTIONS RIGHT PARTNER

8525-209/ EMAIL



Analysis / Test Report

TESTING
No.0042

Client : Dow Chemical Thailand Ltd.
10 Moo 2, Asia Industrial Estate, Tambol Banchang, Amphur Banchang, Rayong Thailand 21130

P/O :

Project Name : Environmental Quality Monitoring

Project Location : AIE_PG Plant

Lot ID: 2518295

Date Received : May 06, 2025

Date Reported : May 20, 2025

Report Number: 3303698-1C16

Page 1 of 1

Sample Number 2518295-6
Parameter Noise (Leq 24 hrs.)
Location บริเวณริมรั้วของโครงการทางด้านทิศตะวันตกของพื้นที่ HPPO (GPS 47P 0726777, 1405417)
Measurement Date May 03 - May 04, 2025
Measurement by Sitpawit Suwannarat
Sound Level meter Serial No. 900071

Time	Leq (dB(A))	Lmax (dB(A))	L90 (dB(A))
12:00 PM - 01:00 PM	58.1	80.3	55.7
01:00 PM - 02:00 PM	57.3	80.4	55.2
02:00 PM - 03:00 PM	58.2	73.1	56.4
03:00 PM - 04:00 PM	60.6	84.4	58.6
04:00 PM - 05:00 PM	60.8	85.9	58.5
05:00 PM - 06:00 PM	59.6	71.9	58.5
06:00 PM - 07:00 PM	60.7	79.7	59.0
07:00 PM - 08:00 PM	59.9	78.1	58.9
08:00 PM - 09:00 PM	59.2	68.0	58.6
09:00 PM - 10:00 PM	59.2	72.1	58.6
10:00 PM - 11:00 PM	59.5	70.6	58.6
11:00 PM - 12:00 AM	60.0	73.2	58.3
12:00 AM - 01:00 AM	60.8	75.7	58.0
01:00 AM - 02:00 AM	59.7	73.4	58.9
02:00 AM - 03:00 AM	61.2	88.6	59.1
03:00 AM - 04:00 AM	60.1	74.5	58.5
04:00 AM - 05:00 AM	59.2	69.1	58.4
05:00 AM - 06:00 AM	60.3	84.4	58.1
06:00 AM - 07:00 AM	61.1	81.1	56.4
07:00 AM - 08:00 AM	61.5	87.1	57.6
08:00 AM - 09:00 AM	62.3	94.1	57.1
09:00 AM - 10:00 AM	58.0	72.6	56.8
10:00 AM - 11:00 AM	58.3	78.7	56.8
11:00 AM - 12:00 PM	57.5	71.0	56.3

Leq Average 24 hrs. (dB(A)) 59.9
Lmax (dB(A)) 94.1
L90 (dB(A)) 58.3
Ldn (dB(A)) 66.6
Standard (dB(A)) 70 115

Reference Method : ISO1996-1 and 1996-2

Standard : 1. ประกาศคณะกรรมการสิ่งแวดล้อมแห่งชาติ ฉบับที่ 15 (พ.ศ. 2540) เรื่องกำหนดมาตรฐานระดับเสียงโดยทั่วไป
2. ประกาศกระทรวงอุตสาหกรรม เรื่องกำหนดค่าระดับเสียงการรบกวน และระดับเสียงที่เกิดจากการประกอบกิจการโรงงาน พ.ศ. 2548

Technical Management

Chontichak

Chonticha Subongkoch

Scientist (3)

Approved by

Supot S

Supot Salamteh

Section Head

The above results are valid only for the analyzed/tested sample(s) as indicated in this report. No part of this report or certificate may be reproduced in any form without written consent from the Laboratory. ALS Laboratory Group (Thailand) strongly recommends that this report is not reproduced except in full.

ADDRESS 616/10 Moo 5 T. Maenam Khu A. Pluakdaeng Rayong 21140 Thailand | PHONE +66 0 3304 8555 | FAX +66 0 3304 8556

Life Sciences

www.alsglobal.com

RIGHT SOLUTIONS RIGHT PARTNER

8525-209/ EMAIL



Analysis / Test Report

TESTING
No.0042

Client : Dow Chemical Thailand Ltd.

10 Moo 2, Asia Industrial Estate, Tambol Banchang, Amphur Banchang, Rayong Thailand
21130

P/O :

Project Name : Environmental Quality Monitoring

Project Location : AIE_PG Plant

Lot ID: 2518300

Date Received : May 06, 2025

Date Reported : May 20, 2025

Report Number: 3303743-1C16

Page 1 of 1

Sample Number	2518300-1
Parameter	Noise (Leq 24 hrs.)
Location	บริเวณริมรั้วของโครงการทางด้านทิศใต้ของพื้นที่ HPPO (ข้างปั๊ม ปรก บล็อก 45) (GPS 47P 0727136, 1404550)
Measurement Date	Apr 28 - Apr 29, 2025
Measurement by	Sitpawit Suwannarat
Sound Level meter	Serial No. 623394

Time	Leq (dB(A))	Lmax (dB(A))	L90 (dB(A))
01:00 PM - 02:00 PM	50.1	76.3	47.1
02:00 PM - 03:00 PM	48.9	64.9	45.6
03:00 PM - 04:00 PM	49.8	70.9	45.6
04:00 PM - 05:00 PM	49.4	69.1	45.5
05:00 PM - 06:00 PM	51.3	78.9	45.6
06:00 PM - 07:00 PM	55.9	86.1	45.1
07:00 PM - 08:00 PM	52.1	73.4	45.1
08:00 PM - 09:00 PM	51.9	74.5	45.8
09:00 PM - 10:00 PM	50.5	72.1	46.0
10:00 PM - 11:00 PM	56.2	73.4	48.0
11:00 PM - 12:00 AM	55.3	77.7	47.7
12:00 AM - 01:00 AM	49.2	66.8	46.5
01:00 AM - 02:00 AM	47.3	67.1	46.3
02:00 AM - 03:00 AM	51.7	65.0	46.6
03:00 AM - 04:00 AM	48.6	59.3	46.3
04:00 AM - 05:00 AM	49.6	58.9	46.3
05:00 AM - 06:00 AM	50.6	71.2	47.4
06:00 AM - 07:00 AM	51.4	80.5	47.6
07:00 AM - 08:00 AM	50.2	69.3	48.2
08:00 AM - 09:00 AM	50.2	70.7	48.5
09:00 AM - 10:00 AM	57.4	79.2	48.9
10:00 AM - 11:00 AM	54.8	81.2	50.1
11:00 AM - 12:00 PM	56.0	77.8	49.5
12:00 PM - 01:00 PM	52.8	79.3	47.5

Leq Average 24 hrs. (dB(A))	52.7		
Lmax (dB(A))		86.1	
L90 (dB(A))			46.5
Ldn (dB(A))	58.6		
Standard (dB(A))	70	115	

Reference Method : ISO1996-1 and 1996-2

Standard : 1. ประกาศคณะกรรมการสิ่งแวดล้อมแห่งชาติ ฉบับที่ 15 (พ.ศ. 2540) เรื่องกำหนดมาตรฐานระดับเสียงโดยทั่วไป
2. ประกาศกระทรวงอุตสาหกรรม เรื่องกำหนดค่าระดับเสียงการรบกวน และระดับเสียงที่เกิดจากการประกอบกิจการ
โรงงาน พ.ศ. 2548

Technical Management

Chontichak

Chonticha Subongkoch

Scientist (3)

Approved by

Supot S

Supot Salamteh

Section Head

The above results are valid only for the analyzed/tested sample(s) as indicated in this report. No part of this report or certificate may be reproduced in any form without written consent from the Laboratory. ALS Laboratory Group (Thailand) strongly recommends that this report is not reproduced except in full.

ADDRESS 616/10 Moo 5 T. Maenam Khu A. Pluakdaeng Rayong 21140 Thailand | PHONE +66 0 3304 8555 | FAX +66 0 3304 8556

Life Sciences

www.alsglobal.com

RIGHT SOLUTIONS RIGHT PARTNER

8525-209/ EMAIL



Analysis / Test Report

TESTING
No.0042

Client : Dow Chemical Thailand Ltd.

10 Moo 2, Asia Industrial Estate, Tambol Banchang, Amphur Banchang, Rayong Thailand 21130

P/O :

Project Name : Environmental Quality Monitoring

Project Location : AIE_PG Plant

Lot ID: 2518300

Date Received : May 06, 2025

Date Reported : May 20, 2025

Report Number: 3303744-1C16

Page 1 of 1

Sample Number 2518300-2
Parameter Noise (Leq 24 hrs.)
Location บริเวณริมรั้วของโครงการทางด้านทิศใต้ของพื้นที่ HPPO (ข้างปั๊ม ปรก บล็อก 45) (GPS 47P 0727136, 1404550)
Measurement Date Apr 29 - Apr 30, 2025
Measurement by Sitpawit Suwannarat
Sound Level meter Serial No. 623394

Time	Leq (dB(A))	Lmax (dB(A))	L90 (dB(A))
01:00 PM - 02:00 PM	54.1	84.7	47.2
02:00 PM - 03:00 PM	51.3	68.2	47.3
03:00 PM - 04:00 PM	51.9	73.3	46.4
04:00 PM - 05:00 PM	53.7	81.7	46.3
05:00 PM - 06:00 PM	48.7	64.4	46.3
06:00 PM - 07:00 PM	52.4	76.7	47.0
07:00 PM - 08:00 PM	52.0	77.0	47.4
08:00 PM - 09:00 PM	53.9	72.9	48.1
09:00 PM - 10:00 PM	51.9	72.6	48.3
10:00 PM - 11:00 PM	57.6	76.8	49.6
11:00 PM - 12:00 AM	58.4	74.7	49.3
12:00 AM - 01:00 AM	50.3	69.4	49.0
01:00 AM - 02:00 AM	51.0	57.7	49.4
02:00 AM - 03:00 AM	50.4	66.0	49.4
03:00 AM - 04:00 AM	53.2	71.7	49.9
04:00 AM - 05:00 AM	57.4	81.0	49.0
05:00 AM - 06:00 AM	50.8	63.5	48.8
06:00 AM - 07:00 AM	51.2	75.9	49.3
07:00 AM - 08:00 AM	49.9	63.8	49.1
08:00 AM - 09:00 AM	52.4	71.8	51.1
09:00 AM - 10:00 AM	57.3	70.7	52.4
10:00 AM - 11:00 AM	56.3	72.6	52.3
11:00 AM - 12:00 PM	56.3	85.1	51.1
12:00 PM - 01:00 PM	56.6	82.5	49.2

Leq Average 24 hrs. (dB(A)) 54.2
Lmax (dB(A)) 85.1
L90 (dB(A)) 49.0
Ldn (dB(A)) 61.0
Standard (dB(A)) 70 115

Reference Method : ISO1996-1 and 1996-2

Standard : 1. ประกาศคณะกรรมการสิ่งแวดล้อมแห่งชาติ ฉบับที่ 15 (พ.ศ. 2540) เรื่องกำหนดมาตรฐานระดับเสียงโดยทั่วไป
2. ประกาศกระทรวงอุตสาหกรรม เรื่องกำหนดค่าระดับเสียงการรบกวน และระดับเสียงที่เกิดจากการประกอบกิจการโรงงาน พ.ศ. 2548

Technical Management

Chontichak

Chonticha Subongkoch
Scientist (3)

Approved by

Supot S

Supot Salamteh
Section Head

The above results are valid only for the analyzed/tested sample(s) as indicated in this report. No part of this report or certificate may be reproduced in any form without written consent from the Laboratory. ALS Laboratory Group (Thailand) strongly recommends that this report is not reproduced except in full.

ADDRESS 616/10 Moo 5 T. Maenam Khu A. Pluakdaeng Rayong 21140 Thailand | PHONE +66 0 3304 8555 | FAX +66 0 3304 8556

Life Sciences

www.alsglobal.com

RIGHT SOLUTIONS RIGHT PARTNER

8525-209/ EMAIL



Analysis / Test Report

TESTING
No.0042

Client : Dow Chemical Thailand Ltd.
10 Moo 2, Asia Industrial Estate, Tambol Banchang, Amphur Banchang, Rayong Thailand 21130

P/O :

Project Name : Environmental Quality Monitoring

Project Location : AIE_PG Plant

Lot ID: 2518300

Date Received : May 06, 2025

Date Reported : May 20, 2025

Report Number: 3303745-1C16

Page 1 of 1

Sample Number 2518300-3
Parameter Noise (Leq 24 hrs.)
Location บริเวณริมรั้วของโครงการทางด้านทิศใต้ของพื้นที่ HPPO (ข้างปั๊ม ปรก บล็อก 45) (GPS 47P 0727136, 1404550)
Measurement Date Apr 30 - May 01, 2025
Measurement by Sitpawit Suwannarat
Sound Level meter Serial No. 623394

Time	Leq (dB(A))	Lmax (dB(A))	L90 (dB(A))
01:00 PM - 02:00 PM	54.9	80.9	47.6
02:00 PM - 03:00 PM	52.3	69.8	47.9
03:00 PM - 04:00 PM	53.8	72.4	47.2
04:00 PM - 05:00 PM	52.0	84.1	46.4
05:00 PM - 06:00 PM	52.5	73.3	46.2
06:00 PM - 07:00 PM	52.1	76.3	45.4
07:00 PM - 08:00 PM	54.6	77.6	46.7
08:00 PM - 09:00 PM	52.4	71.8	45.9
09:00 PM - 10:00 PM	50.5	67.8	46.3
10:00 PM - 11:00 PM	55.8	81.2	48.0
11:00 PM - 12:00 AM	50.9	70.7	46.1
12:00 AM - 01:00 AM	53.0	79.9	46.9
01:00 AM - 02:00 AM	51.1	75.6	47.3
02:00 AM - 03:00 AM	61.5	83.5	49.3
03:00 AM - 04:00 AM	50.8	66.1	48.8
04:00 AM - 05:00 AM	52.7	70.0	49.3
05:00 AM - 06:00 AM	52.5	64.7	49.5
06:00 AM - 07:00 AM	55.7	70.4	48.6
07:00 AM - 08:00 AM	60.3	74.3	50.4
08:00 AM - 09:00 AM	58.1	72.9	51.2
09:00 AM - 10:00 AM	57.2	81.7	52.0
10:00 AM - 11:00 AM	57.7	79.9	53.1
11:00 AM - 12:00 PM	56.6	70.6	51.1
12:00 PM - 01:00 PM	56.2	79.0	49.7

Leq Average 24 hrs. (dB(A)) 55.5
Lmax (dB(A)) 84.1
L90 (dB(A)) 47.9
Ldn (dB(A)) 61.8
Standard (dB(A)) 70 115

Reference Method : ISO1996-1 and 1996-2

Standard : 1. ประกาศคณะกรรมการสิ่งแวดล้อมแห่งชาติ ฉบับที่ 15 (พ.ศ. 2540) เรื่องกำหนดมาตรฐานระดับเสียงโดยทั่วไป
2. ประกาศกระทรวงอุตสาหกรรม เรื่องกำหนดค่าระดับเสียงการรบกวน และระดับเสียงที่เกิดจากการประกอบกิจการโรงงาน พ.ศ. 2548

Technical Management

Chontichak

Chonticha Subongkoch
Scientist (3)

Approved by

Supot S

Supot Salamteh
Section Head

The above results are valid only for the analyzed/tested sample(s) as indicated in this report. No part of this report or certificate may be reproduced in any form without written consent from the Laboratory. ALS Laboratory Group (Thailand) strongly recommends that this report is not reproduced except in full.

ADDRESS 616/10 Moo 5 T. Maenam Khu A. Pluakdaeng Rayong 21140 Thailand | PHONE +66 0 3304 8555 | FAX +66 0 3304 8556

Life Sciences

www.alsglobal.com

RIGHT SOLUTIONS RIGHT PARTNER

8525-209/ EMAIL



Analysis / Test Report

TESTING
No.0042

Client : Dow Chemical Thailand Ltd.

10 Moo 2, Asia Industrial Estate, Tambol Banchang, Amphur Banchang, Rayong Thailand
21130

P/O :

Project Name : Environmental Quality Monitoring

Project Location : AIE_PG Plant

Lot ID: 2518300

Date Received : May 06, 2025

Date Reported : May 20, 2025

Report Number: 3303746-1C16

Page 1 of 1

Sample Number 2518300-4
Parameter Noise (Leq 24 hrs.)
Location บริเวณริมรั้วของโครงการทางด้านทิศใต้ของพื้นที่ HPPO (ข้างปั๊ม รมก บล็อก 45) (GPS 47P 0727136, 1404550)
Measurement Date May 01 - May 02, 2025
Measurement by Sitpawit Suwannarat
Sound Level meter Serial No. 623394

Time	Leq (dB(A))	Lmax (dB(A))	L90 (dB(A))
01:00 PM - 02:00 PM	53.2	67.9	48.1
02:00 PM - 03:00 PM	53.6	63.9	48.5
03:00 PM - 04:00 PM	53.2	72.2	48.4
04:00 PM - 05:00 PM	53.9	68.5	48.4
05:00 PM - 06:00 PM	51.5	70.0	46.3
06:00 PM - 07:00 PM	55.4	67.4	49.3
07:00 PM - 08:00 PM	52.5	69.1	47.8
08:00 PM - 09:00 PM	54.3	71.4	48.8
09:00 PM - 10:00 PM	55.0	74.7	49.8
10:00 PM - 11:00 PM	57.1	69.5	51.8
11:00 PM - 12:00 AM	53.3	71.1	49.6
12:00 AM - 01:00 AM	52.9	66.8	49.2
01:00 AM - 02:00 AM	56.4	66.8	50.1
02:00 AM - 03:00 AM	53.5	70.8	49.7
03:00 AM - 04:00 AM	57.6	79.1	50.3
04:00 AM - 05:00 AM	54.9	66.9	51.7
05:00 AM - 06:00 AM	52.5	64.3	50.6
06:00 AM - 07:00 AM	52.5	73.0	49.3
07:00 AM - 08:00 AM	55.3	77.7	48.9
08:00 AM - 09:00 AM	52.3	73.5	49.0
09:00 AM - 10:00 AM	56.5	79.4	49.6
10:00 AM - 11:00 AM	54.7	77.9	49.9
11:00 AM - 12:00 PM	54.0	79.3	49.0
12:00 PM - 01:00 PM	54.7	81.8	47.1

Leq Average 24 hrs. (dB(A)) 54.5
Lmax (dB(A)) 81.8
L90 (dB(A)) 49.2
Ldn (dB(A)) 61.3
Standard (dB(A)) 70 115

Reference Method : ISO1996-1 and 1996-2

Standard : 1. ประกาศคณะกรรมการสิ่งแวดล้อมแห่งชาติ ฉบับที่ 15 (พ.ศ. 2540) เรื่องกำหนดมาตรฐานระดับเสียงโดยทั่วไป
2. ประกาศกระทรวงอุตสาหกรรม เรื่องกำหนดค่าระดับเสียงการรบกวน และระดับเสียงที่เกิดจากการประกอบกิจการ
โรงงาน พ.ศ. 2548

Technical Management

Chontichak

Chonticha Subongkoch
Scientist (3)

Approved by

Suppt S

Supot Salamteh
Section Head

The above results are valid only for the analyzed/tested sample(s) as indicated in this report. No part of this report or certificate may be reproduced in any form without written consent from the Laboratory. ALS Laboratory Group (Thailand) strongly recommends that this report is not reproduced except in full.

ADDRESS 616/10 Moo 5 T. Maenam Khu A. Pluakdaeng Rayong 21140 Thailand | PHONE +66 0 3304 8555 | FAX +66 0 3304 8556

Life Sciences

www.alsglobal.com

RIGHT SOLUTIONS RIGHT PARTNER

8525-209/ EMAIL



Analysis / Test Report

TESTING
No.0042

Client : Dow Chemical Thailand Ltd.
10 Moo 2, Asia Industrial Estate, Tambol Banchang, Amphur Banchang, Rayong Thailand 21130

P/O :

Project Name : Environmental Quality Monitoring

Project Location : AIE_PG Plant

Lot ID: 2518300

Date Received : May 06, 2025

Date Reported : May 20, 2025

Report Number: 3303747-1C16

Page 1 of 1

Sample Number 2518300-5
Parameter Noise (Leq 24 hrs.)
Location บริเวณริมรั้วของโครงการทางด้านทิศใต้ของพื้นที่ HPPO (ข้างปั๊ม ปรก บล็อก 45) (GPS 47P 0727136, 1404550)
Measurement Date May 02 - May 03, 2025
Measurement by Sitpawit Suwannarat
Sound Level meter Serial No. 623394

Time	Leq (dB(A))	Lmax (dB(A))	L90 (dB(A))
01:00 PM - 02:00 PM	53.4	69.4	48.0
02:00 PM - 03:00 PM	53.8	79.5	48.6
03:00 PM - 04:00 PM	54.3	78.9	45.8
04:00 PM - 05:00 PM	52.7	72.9	47.0
05:00 PM - 06:00 PM	49.7	70.0	46.4
06:00 PM - 07:00 PM	55.7	79.6	48.2
07:00 PM - 08:00 PM	51.0	72.8	47.2
08:00 PM - 09:00 PM	49.5	66.7	46.7
09:00 PM - 10:00 PM	49.7	67.2	46.9
10:00 PM - 11:00 PM	51.5	65.5	46.8
11:00 PM - 12:00 AM	46.5	56.3	45.6
12:00 AM - 01:00 AM	50.9	62.3	45.5
01:00 AM - 02:00 AM	53.2	81.6	45.7
02:00 AM - 03:00 AM	58.4	81.4	49.2
03:00 AM - 04:00 AM	57.9	83.2	52.0
04:00 AM - 05:00 AM	59.2	80.4	52.8
05:00 AM - 06:00 AM	61.9	73.2	52.5
06:00 AM - 07:00 AM	56.0	77.5	51.4
07:00 AM - 08:00 AM	53.9	73.7	50.5
08:00 AM - 09:00 AM	52.9	74.9	49.3
09:00 AM - 10:00 AM	55.7	85.6	48.5
10:00 AM - 11:00 AM	56.6	72.4	48.2
11:00 AM - 12:00 PM	50.9	76.5	47.5
12:00 PM - 01:00 PM	53.3	68.2	47.4

Leq Average 24 hrs. (dB(A)) 55.2
Lmax (dB(A)) 85.6
L90 (dB(A)) 47.5
Ldn (dB(A)) 63.1
Standard (dB(A)) 70 115

Reference Method : ISO1996-1 and 1996-2

Standard : 1. ประกาศคณะกรรมการสิ่งแวดล้อมแห่งชาติ ฉบับที่ 15 (พ.ศ. 2540) เรื่องกำหนดมาตรฐานระดับเสียงโดยทั่วไป
2. ประกาศกระทรวงอุตสาหกรรม เรื่องกำหนดค่าระดับเสียงการรบกวน และระดับเสียงที่เกิดจากการประกอบกิจการโรงงาน พ.ศ. 2548

Technical Management

Chontichak

Chonticha Subongkoch
Scientist (3)

Approved by

Supot S

Supot Salamteh
Section Head

The above results are valid only for the analyzed/tested sample(s) as indicated in this report. No part of this report or certificate may be reproduced in any form without written consent from the Laboratory. ALS Laboratory Group (Thailand) strongly recommends that this report is not reproduced except in full.

ADDRESS 616/10 Moo 5 T. Maenam Khu A. Pluakdaeng Rayong 21140 Thailand | PHONE +66 0 3304 8555 | FAX +66 0 3304 8556

Life Sciences

www.alsglobal.com

RIGHT SOLUTIONS RIGHT PARTNER

8525-209/ EMAIL



Analysis / Test Report

TESTING
No.0042

Client : Dow Chemical Thailand Ltd.
10 Moo 2, Asia Industrial Estate, Tambol Banchang, Amphur Banchang, Rayong Thailand
21130

P/O :

Project Name : Environmental Quality Monitoring

Project Location : AIE_PG Plant

Lot ID: 2518300

Date Received : May 06, 2025

Date Reported : May 20, 2025

Report Number: 3303748-1C16

Page 1 of 1

Sample Number 2518300-6
Parameter Noise (Leq 24 hrs.)
Location บริเวณริมรั้วของโครงการทางด้านทิศใต้ของพื้นที่ HPPO (ข้างปั๊ม ปรก บล็อก 45) (GPS 47P 0727136, 1404550)
Measurement Date May 03 - May 04, 2025
Measurement by Sitpawit Suwannarat
Sound Level meter Serial No. 623394

Time	Leq (dB(A))	Lmax (dB(A))	L90 (dB(A))
01:00 PM - 02:00 PM	50.6	71.1	48.5
02:00 PM - 03:00 PM	50.8	69.3	48.4
03:00 PM - 04:00 PM	59.0	90.3	50.3
04:00 PM - 05:00 PM	54.9	68.6	52.8
05:00 PM - 06:00 PM	53.5	69.2	51.9
06:00 PM - 07:00 PM	57.1	75.3	52.9
07:00 PM - 08:00 PM	53.6	70.1	51.6
08:00 PM - 09:00 PM	51.5	68.1	50.1
09:00 PM - 10:00 PM	51.7	65.6	49.2
10:00 PM - 11:00 PM	54.8	69.7	49.4
11:00 PM - 12:00 AM	53.9	77.1	49.4
12:00 AM - 01:00 AM	58.4	81.4	49.2
01:00 AM - 02:00 AM	58.5	72.0	51.1
02:00 AM - 03:00 AM	61.1	73.3	51.8
03:00 AM - 04:00 AM	64.4	72.7	51.3
04:00 AM - 05:00 AM	56.4	74.9	50.5
05:00 AM - 06:00 AM	59.8	82.9	51.0
06:00 AM - 07:00 AM	60.8	83.6	49.8
07:00 AM - 08:00 AM	58.5	77.0	52.4
08:00 AM - 09:00 AM	53.7	72.0	50.8
09:00 AM - 10:00 AM	57.0	80.3	50.4
10:00 AM - 11:00 AM	52.4	73.0	49.5
11:00 AM - 12:00 PM	52.7	70.3	48.9
12:00 PM - 01:00 PM	53.7	76.1	46.7

Leq Average 24 hrs. (dB(A)) 57.4
Lmax (dB(A)) 90.3
L90 (dB(A)) 50.3
Ldn (dB(A)) 65.8
Standard (dB(A)) 70 115

Reference Method : ISO1996-1 and 1996-2

Standard : 1. ประกาศคณะกรรมการสิ่งแวดล้อมแห่งชาติ ฉบับที่ 15 (พ.ศ. 2540) เรื่องกำหนดมาตรฐานระดับเสียงโดยทั่วไป
2. ประกาศกระทรวงอุตสาหกรรม เรื่องกำหนดค่าระดับเสียงการรบกวน และระดับเสียงที่เกิดจากการประกอบกิจการ
โรงงาน พ.ศ. 2548

Technical Management

Chontichak

Chonticha Subongkoch
Scientist (3)

Approved by

Supot S

Supot Salamteh
Section Head

The above results are valid only for the analyzed/tested sample(s) as indicated in this report. No part of this report or certificate may be reproduced in any form without written consent from the Laboratory. ALS Laboratory Group (Thailand) strongly recommends that this report is not reproduced except in full.

ADDRESS 616/10 Moo 5 T. Maenam Khu A. Pluakdaeng Rayong 21140 Thailand | PHONE +66 0 3304 8555 | FAX +66 0 3304 8556

Life Sciences

www.alsglobal.com

RIGHT SOLUTIONS RIGHT PARTNER

8525-209/ EMAIL



Analysis / Test Report

TESTING
No.0042

Client : Dow Chemical Thailand Ltd.
10 Moo 2, Asia Industrial Estate, Tambol Banchang, Amphur Banchang, Rayong Thailand 21130

P/O :

Project Name : Environmental Quality Monitoring

Project Location : AIE_PG Plant

Lot ID: 2518300

Date Received : May 06, 2025

Date Reported : May 20, 2025

Report Number: 3303749-1C16

Page 1 of 1

Sample Number 2518300-7
Parameter Noise (Leq 24 hrs.)
Location บริเวณริมรั้วของโครงการทางด้านทิศใต้ของพื้นที่ HPPO (ข้างปั๊ม ปรก บล็อก 45) (GPS 47P 0727136, 1404550)
Measurement Date May 04 - May 05, 2025
Measurement by Sitpawit Suwannarat
Sound Level meter Serial No. 623394

Time	Leq (dB(A))	Lmax (dB(A))	L90 (dB(A))
01:00 PM - 02:00 PM	50.2	69.1	46.1
02:00 PM - 03:00 PM	54.5	73.0	46.1
03:00 PM - 04:00 PM	51.6	78.8	46.8
04:00 PM - 05:00 PM	49.9	66.7	46.8
05:00 PM - 06:00 PM	50.4	65.9	47.3
06:00 PM - 07:00 PM	56.7	70.3	49.8
07:00 PM - 08:00 PM	52.6	71.9	49.0
08:00 PM - 09:00 PM	50.4	72.8	48.2
09:00 PM - 10:00 PM	50.6	61.0	48.5
10:00 PM - 11:00 PM	50.0	65.7	48.7
11:00 PM - 12:00 AM	51.0	75.4	48.6
12:00 AM - 01:00 AM	49.8	62.6	48.3
01:00 AM - 02:00 AM	54.6	69.8	47.8
02:00 AM - 03:00 AM	53.8	81.9	47.6
03:00 AM - 04:00 AM	56.1	78.5	48.0
04:00 AM - 05:00 AM	50.0	68.5	47.8
05:00 AM - 06:00 AM	57.6	67.2	48.5
06:00 AM - 07:00 AM	53.3	74.4	49.9
07:00 AM - 08:00 AM	52.0	68.6	48.8
08:00 AM - 09:00 AM	53.7	77.5	46.8
09:00 AM - 10:00 AM	50.7	76.2	46.4
10:00 AM - 11:00 AM	52.6	79.5	46.7
11:00 AM - 12:00 PM	52.6	72.2	46.0
12:00 PM - 01:00 PM	48.9	68.6	45.5

Leq Average 24 hrs. (dB(A)) 52.9
Lmax (dB(A)) 81.9
L90 (dB(A)) 47.8
Ldn (dB(A)) 60.0
Standard (dB(A)) 70 115

Reference Method : ISO1996-1 and 1996-2

Standard : 1. ประกาศคณะกรรมการสิ่งแวดล้อมแห่งชาติ ฉบับที่ 15 (พ.ศ. 2540) เรื่องกำหนดมาตรฐานระดับเสียงโดยทั่วไป
2. ประกาศกระทรวงอุตสาหกรรม เรื่องกำหนดค่าระดับเสียงการรบกวน และระดับเสียงที่เกิดจากการประกอบกิจการโรงงาน พ.ศ. 2548

Technical Management

Chontichak

Chonticha Subongkoch
Scientist (3)

Approved by

Supot S

Supot Salamteh
Section Head

The above results are valid only for the analyzed/tested sample(s) as indicated in this report. No part of this report or certificate may be reproduced in any form without written consent from the Laboratory. ALS Laboratory Group (Thailand) strongly recommends that this report is not reproduced except in full.

ADDRESS 616/10 Moo 5 T. Maenam Khu A. Pluakdaeng Rayong 21140 Thailand | PHONE +66 0 3304 8555 | FAX +66 0 3304 8556

Life Sciences

www.alsglobal.com

RIGHT SOLUTIONS RIGHT PARTNER

8525-209/ EMAIL

ภาคผนวก ค-4

ผลการตรวจวิเคราะห์คุณภาพน้ำเสียจากกระบวนการผลิต



Analysis / Test Report

TESTING
No.0042

Client : Dow Chemical Thailand Ltd.
10 Moo 2, Asia Industrial Estate, Tambol Banchang, Amphur Banchang, Rayong Thailand
21130

P/O :
Project Name : Water Testing
Project Location : AIE_PG Plant

Lot ID: 24143086

Date Received : Jan 08, 2025
Date Reported : Jan 16, 2025
Report Number : 3215073-1

Page 1 of 1

Sample Number 24143086-1
Sampled Date Jan 08, 2025 11:15 AM
Sample Description Wastewater
Location PG Process
Date Analysis Commenced Jan 08, 2025
Condition of Sample Contained in two glass vials, three amber glass bottles and three plastic bottles. Sample containers comply to pretreatment - preservation standards (APHA / USEPA)

Analyte	Unit	LOD	LOQ (LOR)	Result	Method	Testing Location
Water Testing						
BOD (5 days at 20 Degree C)	mg/L	-	2.0	3065	Standard Methods for the Examination of Water and Wastewater. APHA, AWWA & WEF, 24th ed., 2023, part 5210 B, part 4500 - O G	Rayong
COD	mg/L	1.5	25	20227	Standard Methods for the Examination of Water and Wastewater. APHA, AWWA & WEF, 24th ed., 2023, part 5220 D	Rayong
Oil & Grease	mg/L	-	3	<3	Standard Methods for the Examination of Water and Wastewater. APHA, AWWA & WEF, 24th ed., 2023, part 5520 B	Rayong
pH at 25 degree C		-	-	4.2	Standard Methods for the Examination of Water and Wastewater. APHA, AWWA & WEF, 24th ed., 2023, part 4500 - H (B)	Rayong
Total Suspended Solids Dried at 103-105 degree C	mg/L	-	5	<5	Standard Methods for the Examination of Water and Wastewater. APHA, AWWA & WEF, 24th ed., 2023, part 2540 D	Rayong

Sampling By : Wanlop Hunchainaow ทะเบียนเลขที่ ว-323-จ-0038 , Pattarapol Sawangjaitam ทะเบียนเลขที่ ว-204-จ-0002

Remark :
- LOD : Limit of Detection
- "<" : Lower than LOQ (Limit of Quantitation) / LOR (Limit of Reporting)
- Analyte(s) marked * is/are not included in scope of Accreditation ISO/IEC 17025.
- The laboratory has been accepted as an accredited laboratory complying with the ISO/IEC 17025.

Technical Management

Photchana S.

Photchana Seeda
Scientist (4)

ทะเบียนเลขที่ ว-323-จ-0028

Approved by

D. Changchon.

Dej Changchon
Senior Manager

ทะเบียนเลขที่ ว-323-ค-0001

Results apply to the sample(s) as submitted, unless the sampling was conducted by ALS. No part of this report may be reproduced in any form without written consent from the laboratory.
ALS Laboratory Group (Thailand) strongly recommends that this report is not reproduced except in full.

ADDRESS 616/10 Moo 5 T. Maenam Khu A. Pluakdaeng Rayong 21140 Thailand | PHONE +66 0 3304 8555 | FAX +66 0 3304 8556
ALS LABORATORY GROUP (THAILAND) CO., LTD. An ALS Limited Company

Life Sciences

www.alsglobal.com

RIGHT SOLUTIONS RIGHT PARTNER



Analysis / Test Report

Client : Dow Chemical Thailand Ltd.
10 Moo 2, Asia Industrial Estate, Tambol Banchang, Amphur Banchang, Rayong Thailand
21130

P/O :
Project Name : Water Testing
Project Location : AIE_PG Plant

Lot ID: 24143086

Date Received : Jan 08, 2025
Date Reported : Jan 16, 2025
Report Number : 3215073-2

Page 1 of 1

Sample Number 24143086-1
Sampled Date Jan 08, 2025 11:15 AM
Sample Description Wastewater
Location PG Process
Date Analysis Commenced Jan 09, 2025
Condition of Sample Contained in two glass vials, three amber glass bottles and three plastic bottles. Sample containers comply to pretreatment - preservation standards (APHA / USEPA)

Analyte	Unit	LOD	LOQ (LOR)	Result	Method	Testing Location
Water Testing						
Propylene Glycol	mg/L	-	1.0	6476	In-house method based on United States Environmental Protection Agency, EPA Method 8015 B	Bangkok
Total Organic Carbon	mg/L	0.01	0.1	5090	Standard Methods for the Examination of Water and Wastewater. APHA, AWWA & WEF, 24th ed., 2023, part 5310 B	Bangkok

Sampling By : Wanlop Hunchainaw , Pattarapol Sawangjaitam

Remark :

- LOD : Limit of Detection
- "<" : Lower than LOQ (Limit of Quantitation) / LOR (Limit of Reporting)

Approved by

Siriluk P.

Siriluk Bunnak
Section Head

Results apply to the sample(s) as submitted, unless the sampling was conducted by ALS. No part of this report may be reproduced in any form without written consent from the laboratory. ALS Laboratory Group (Thailand) strongly recommends that this report is not reproduced except in full.

ADDRESS 104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan, Khet Suan Luang, Bangkok 10250 Thailand | PHONE +66 0 2760 3000 | FAX +66 0 2760 3197
ALS LABORATORY GROUP (THAILAND) CO., LTD. An ALS Limited Company

Life Sciences

www.alsglobal.com

RIGHT SOLUTIONS RIGHT PARTNER

8525-71/ EMAIL

S:\Reports\MixRef_All_NoGL.rpt (11:04AM)



Analysis / Test Report

TESTING
No.0042

Client : Dow Chemical Thailand Ltd.
10 Moo 2, Asia Industrial Estate, Tambol Banchang, Amphur Banchang, Rayong Thailand
21130
P/O : 4516938822
Project Name : Water Testing
Project Location : AIE_PG Plant

Lot ID: 255322

Date Received : Feb 05, 2025
Date Reported : Feb 14, 2025
Report Number : 3234669-1

Page 1 of 1

Sample Number 255322-1
Sampled Date Feb 05, 2025 11:05 AM
Sample Description Wastewater
Location PG Process
Date Analysis Commenced Feb 05, 2025
Condition of Sample Contained in three amber glass bottles, two glass vials and three plastic bottles, sample containers comply to pretreatment - preservation standards (APHA, USEPA)

Analyte	Unit	LOD	LOQ (LOR)	Result	Method	Testing Location
Water Testing						
BOD (5 days at 20 Degree C)	mg/L	-	2.0	1295	Standard Methods for the Examination of Water and Wastewater. APHA, AWWA & WEF, 24th ed., 2023, part 5210 B, part 4500 - O G	Rayong
COD *	mg/L	1.5	25	27951	Standard Methods for the Examination of Water and Wastewater. APHA, AWWA & WEF, 24th ed., 2023, part 5220 D	Rayong
Oil & Grease	mg/L	-	3	<3	Standard Methods for the Examination of Water and Wastewater. APHA, AWWA & WEF, 24th ed., 2023, part 5520 B	Rayong
pH at 25 degree C *		-	-	3.9	Standard Methods for the Examination of Water and Wastewater. APHA, AWWA & WEF, 24th ed., 2023, part 4500 - H (B)	Rayong
Total Suspended Solids Dried at 103-105 degree C	mg/L	-	5	<5	Standard Methods for the Examination of Water and Wastewater. APHA, AWWA & WEF, 24th ed., 2023, part 2540 D	Rayong

Sampling By : Sansoen Khuiyoksui ทะเบียนเลขที่ ว-323-จ-0005 , Pattarapol Sawangjaitam ทะเบียนเลขที่ ว-204-จ-0002

Remark :

- LOD : Limit of Detection
- "<" : Lower than LOQ (Limit of Quantitation) / LOR (Limit of Reporting)
- Analyte(s) marked * is/are not included in scope of Accreditation ISO/IEC 17025.

Technical Management

Photchana S.

Photchana Seeda
Scientist (4)

ทะเบียนเลขที่ ว-323-จ-0028

Approved by

D. Chamon.

Dej Changchon
Senior Manager

ทะเบียนเลขที่ ว-323-ค-0001

Results apply to the sample(s) as submitted, unless the sampling was conducted by ALS. The report shall not be reproduced except in full without the written approval of the laboratory.

ADDRESS 616/10 Moo 5 T. Maenam Khu A. Pluakdaeng Rayong 21140 Thailand | PHONE +66 0 3304 8555 | FAX +66 0 3304 8556
ALS LABORATORY GROUP (THAILAND) CO., LTD. An ALS Limited Company

Life Sciences

www.alsglobal.com

RIGHT SOLUTIONS RIGHT PARTNER



Analysis / Test Report

Client : Dow Chemical Thailand Ltd.
10 Moo 2, Asia Industrial Estate, Tambol Banchang, Amphur Banchang, Rayong Thailand
21130
P/O : 4516938822
Project Name : Water Testing
Project Location : AIE_PG Plant

Lot ID: 255322

Date Received : Feb 05, 2025
Date Reported : Feb 14, 2025
Report Number : 3234669-2

Page 1 of 1

Sample Number 255322-1
Sampled Date Feb 05, 2025 11:05 AM
Sample Description Wastewater
Location PG Process
Date Analysis Commenced Feb 06, 2025
Condition of Sample Contained in three amber glass bottles, two glass vials and three plastic bottles, sample containers comply to pretreatment - preservation standards (APHA, USEPA)

Analyte	Unit	LOD	LOQ (LOR)	Result	Method	Testing Location
Water Testing						
Propylene Glycol	mg/L	-	1.0	7791	In-house method based on United States Environmental Protection Agency, EPA Method 8015 B	Bangkok
Total Organic Carbon	mg/L	0.01	0.1	6186	Standard Methods for the Examination of Water and Wastewater. APHA, AWWA & WEF, 24th ed., 2023, part 5310 B	Bangkok

Sampling By : Sansoen Khuiyoksui , Pattarapol Sawangjaitam

Remark :

- LOD : Limit of Detection
- "<" : Lower than LOQ (Limit of Quantitation) / LOR (Limit of Reporting)

Approved by

Siriluk P.

Siriluk Bunnak
Section Head

Results apply to the sample(s) as submitted, unless the sampling was conducted by ALS. The report shall not be reproduced except in full without the written approval of the laboratory.



Analysis / Test Report

TESTING
No.0042

Client : Dow Chemical Thailand Ltd.
10 Moo 2, Asia Industrial Estate, Tambol Banchang, Amphur Banchang, Rayong Thailand
21130
P/O : 4516938822
Project Name : Water Testing
Project Location : AIE_PG Plant

Lot ID: 2527496

Date Received : Apr 23, 2025
Date Reported : Apr 30, 2025
Report - umber : 3294969v1

Page 1 of 1

Sample Number 252f 496v1
Sampled Date Apr 23, 2025 10:50 AM
Sample Description Wastewater
Location PG Process
Date Analysis Commenced Apr 23, 2025
Condition of Sample Contained in two glass Fials, three amber glass bottles and three plastic bottles, sample containers comply to pretreatment v
preserFation standards (APHA, USEPA)

Analyte	Unit	LOD	LOQ (LOR)	Result	Method	Testing Location
Water Testing						
BOD (5 days at 20 Degree C)	mg/L	v	2.0	1446	Standard Methods for the Examination of Water and Wastewater. APHA, AWWA & WE*, 24th ed., 2023, part 5210 B, part 4500 v O G	Rayong
COD	mg/L	1.5	25	15f 99	Standard Methods for the Examination of Water and Wastewater. APHA, AWWA & WE*, 24th ed., 2023, part 5220 D	Rayong
Oil & Grease	mg/L	v	3	7 3	Standard Methods for the Examination of Water and Wastewater. APHA, AWWA & WE*, 24th ed., 2023, part 5520 B	Rayong
pH at 25 degree C		v	v	4.2	Standard Methods for the Examination of Water and Wastewater. APHA, AWWA & WE*, 24th ed., 2023, part 4500 v H (B)	Rayong
Total Suspended Solids Dried at 103v105 degree C	mg/L	v	5	7 5	Standard Methods for the Examination of Water and Wastewater. APHA, AWWA & WE*, 24th ed., 2023, part 2540 D	Rayong

Sampling By : Sansoen <huiyoKsui ทะเบียนเลขที่ ว323จว0005

Remark :

- LOD : Limit of Detection
- j7j : Lower than LOD (Limit of Quantitation) / LOR (Limit of Reporting)
- Analyte(s) marked Q is/are not included in scope of Accreditation ISO/IEC 17025.
- Sampling is not included in scope of Accreditation ISO/IEC 17025

Technical Management

Photchana S.

Photchana Seeda
Scientist (4)

ทะเบียนเลขที่ ว323จว0028

Approved by

D. Chamon.

De" Changchon
Senior Manager

ทะเบียนเลขที่ ว323จว0001

Results apply to the sample(s) as submitted, unless the sampling was conducted by ALS. The report shall not be reproduced except in full without the written approval of the laboratory.

ADDRESS 616/10 Moo 5 T. Maenam Khu A. Pluakdaeng Rayong 21140 Thailand | PHONE +66 0 3304 8555 | FAX +66 0 3304 8556
ALS LABORATORY GROUP (THAILAND) CO., LTD. An ALS Limited Company

Life Sciences

www.alsglobal.com

RIGHT SOLUTIONS RIGHT PARTNER



Analysis / Test Report

Client : Dow Chemical Thailand Ltd.
10 Moo 2, Asia Industrial Estate, Tambol Banchang, Amphur Banchang, Rayong Thailand
21130
P/O : 4516938822
Project Name : Water Testing
Project Location : AIE_PG Plant

Lot ID: 2527496

Date Received : Apr 23, 2025
Date Reported : May 02, 2025
Report Number : 3294969-2

Page 1 of 1

Sample Number 2527496-1
Sampled Date Apr 23, 2025 10:50 AM
Sample Description Wastewater
Location PG Process
Date Analysis Commenced Apr 24, 2025
Condition of Sample Contained in two glass vials, three amber glass bottles and three plastic bottles, sample containers comply to pretreatment - preservation standards (APHA, USEPA)

Analyte	Unit	LOD	LOQ (LOR)	Result	Method	Testing Location
Water Testing						
Propylene Glycol	mg/L	-	1.0	7398	In-house method based on United States Environmental Protection Agency, EPA Method 8015 B	Bangkok
Total Organic Carbon	mg/L	0.01	0.1	4193	Standard Methods for the Examination of Water and Wastewater. APHA, AWWA & WEF, 24th ed., 2023, part 5310 B	Bangkok

Sampling By : Sansoen Khuiyoksui

Remark :

- LOD : Limit of Detection
- "<" : Lower than LOQ (Limit of Quantitation) / LOR (Limit of Reporting)

Approved by

Siriluk P.

Siriluk Bunnak
Section Head

Results apply to the sample(s) as submitted, unless the sampling was conducted by ALS. The report shall not be reproduced except in full without the written approval of the laboratory.



Analysis / Test Report

TESTING
No.0042

Client : Dow Chemical Thailand Ltd.
10 Moo 2, Asia Industrial Estate, Tambol Banchang, Amphur Banchang, Rayong Thailand
21130
P/O : 4516938822
Project Name : Water Testing
Project Location : AIE_PG Plant

Lot ID: 2539224

Date Received : May 07, 2025
Date Reported : May 16, 2025
Report Number : 3307022-1

Page 1 of 1

Sample Number 2539224-1
Sampled Date May 07, 2025 11:18 AM
Sample Description Wastewater
Location PG Process
Date Analysis Commenced May 07, 2025
Condition of Sample Contained in two glass vials, two amber glass bottles and three plastic bottles, sample containers comply to pretreatment - preservation standards (APHA, USEPA)

Analyte	Unit	LOD	LOQ (LOR)	Result	Method	Testing Location
Water Testing						
BOD (5 days at 20 Degree C)	mg/L	-	2.0	6663	Standard Methods for the Examination of Water and Wastewater. APHA, AWWA & WEF, 24th ed., 2023, part 5210 B, part 4500 - O G	Rayong
COD	mg/L	1.5	25	41041	Standard Methods for the Examination of Water and Wastewater. APHA, AWWA & WEF, 24th ed., 2023, part 5220 D	Rayong
Oil & Grease	mg/L	-	3	<3	Standard Methods for the Examination of Water and Wastewater. APHA, AWWA & WEF, 24th ed., 2023, part 5520 B	Rayong
pH at 25 degree C		-	-	3.9	Standard Methods for the Examination of Water and Wastewater. APHA, AWWA & WEF, 24th ed., 2023, part 4500 - H (B)	Rayong
Total Suspended Solids Dried at 103-105 degree C	mg/L	-	5	<5	Standard Methods for the Examination of Water and Wastewater. APHA, AWWA & WEF, 24th ed., 2023, part 2540 D	Rayong

Sampling By : Surawit Narapong ทะเบียนเลขที่ ว-323-จ-0011 , Pattarapol Sawangjaitam ทะเบียนเลขที่ ว-204-จ-0002

Remark :

- LOD : Limit of Detection
- "<" : Lower than LOQ (Limit of Quantitation) / LOR (Limit of Reporting)
- Analyte(s) marked * is/are not included in scope of Accreditation ISO/IEC 17025.
- Sampling is not included in scope of accreditation ISO/IEC 17025

Technical Management

Photchana S.

Photchana Seeda
Scientist (4)

ทะเบียนเลขที่ ว-323-จ-0028

Approved by

D. Chamon.

Dej Changchon
Senior Manager

ทะเบียนเลขที่ ว-323-ค-0001

Results apply to the sample(s) as submitted, unless the sampling was conducted by ALS. The report shall not be reproduced except in full without the written approval of the laboratory.

ADDRESS 616/10 Moo 5 T. Maenam Khu A. Pluakdaeng Rayong 21140 Thailand | PHONE +66 0 3304 8555 | FAX +66 0 3304 8556
ALS LABORATORY GROUP (THAILAND) CO., LTD. An ALS Limited Company

Life Sciences

www.alsglobal.com

RIGHT SOLUTIONS RIGHT PARTNER



Analysis / Test Report

Client : Dow Chemical Thailand Ltd.
10 Moo 2, Asia Industrial Estate, Tambol Banchang, Amphur Banchang, Rayong Thailand
21130
P/O : 4516938822
Project Name : Water Testing
Project Location : AIE_PG Plant

Lot ID: 2539224

Date Received : May 07, 2025
Date Reported : May 16, 2025
Report Number : 3307022-2

Page 1 of 1

Sample Number 2539224-1
Sampled Date May 07, 2025 11:18 AM
Sample Description Wastewater
Location PG Process
Date Analysis Commenced May 08, 2025
Condition of Sample Contained in two glass vials, two amber glass bottles and three plastic bottles, sample containers comply to pretreatment - preservation standards (APHA, USEPA)

Analyte	Unit	LOD	LOQ (LOR)	Result	Method	Testing Location
Water Testing						
Propylene Glycol	mg/L	-	1.0	9323	In-house method based on United States Environmental Protection Agency, EPA Method 8015 B	Bangkok
Total Organic Carbon	mg/L	0.01	0.1	6346	Standard Methods for the Examination of Water and Wastewater. APHA, AWWA & WEF, 24th ed., 2023, part 5310 B	Bangkok

Sampling By : Surawit Narapong , Pattarapol Sawangjaitam

Remark :

- LOD : Limit of Detection
- "<" : Lower than LOQ (Limit of Quantitation) / LOR (Limit of Reporting)

Approved by

Suwimon C.

Suwimon Chairuangwut
Scientist (3)

Results apply to the sample(s) as submitted, unless the sampling was conducted by ALS. The report shall not be reproduced except in full without the written approval of the laboratory.



Analysis / Test Report

TESTING
No.0042

Client : Dow Chemical Thailand Ltd.
10 Moo 2, Asia Industrial Estate, Tambol Banchang, Amphur Banchang, Rayong Thailand
21130
P/O : 4516938822
Project Name : Water Testing
Project Location : AIE_PG Plant

Lot ID: 2549530

Date Received : Jun 04, 2025
Date Reported : Jun 12, 2025
Report Number : 3332393-1

Page 1 of 1

Sample Number 2549530-1
Sampled Date Jun 04, 2025 10:30 AM
Sample Description Wastewater
Location PG Process
Date Analysis Commenced Jun 04, 2025
Condition of Sample Contained in two glass vials, three amber glass bottles and three plastic bottles, sample containers comply to pretreatment - preservation standards (APHA, USEPA)

Analyte	Unit	LOD	LOQ (LOR)	Result	Method	Testing Location
Water Testing						
BOD (5 days at 20 Degree C)	mg/L	-	2.0	6372	Standard Methods for the Examination of Water and Wastewater. APHA, AWWA & WEF, 24th ed., 2023, part 5210 B, part 4500 - O G	Rayong
COD *	mg/L	1.5	25	39668	Standard Methods for the Examination of Water and Wastewater. APHA, AWWA & WEF, 24th ed., 2023, part 5220 D	Rayong
Oil & Grease	mg/L	-	3	<3	Standard Methods for the Examination of Water and Wastewater. APHA, AWWA & WEF, 24th ed., 2023, part 5520 B	Rayong
pH at 25 degree C		-	-	4.0	Standard Methods for the Examination of Water and Wastewater. APHA, AWWA & WEF, 24th ed., 2023, part 4500 - H (B)	Rayong
Total Suspended Solids Dried at 103-105 degree C	mg/L	-	5	<5	Standard Methods for the Examination of Water and Wastewater. APHA, AWWA & WEF, 24th ed., 2023, part 2540 D	Rayong

Sampling By : Amonwich Wongsachai ทะเบียนเลขที่ ว-323-จ-0040 , Pattarapol Sawangjaitam ทะเบียนเลขที่ ว-204-จ-0002

Remark :

- LOD : Limit of Detection
- "<" : Lower than LOQ (Limit of Quantitation) / LOR (Limit of Reporting)
- Analyte(s) marked * is/are not included in scope of Accreditation ISO/IEC 17025.
- Sampling is not included in scope of accreditation ISO/IEC 17025

Technical Management

Photchana S.

Photchana Seeda
Scientist (4)

ทะเบียนเลขที่ ว-323-จ-0028

Approved by

D. Chamon.

Dej Changchon
Senior Manager

ทะเบียนเลขที่ ว-323-ค-0001

Results apply to the sample(s) as submitted, unless the sampling was conducted by ALS. The report shall not be reproduced except in full without the written approval of the laboratory.

ADDRESS 616/10 Moo 5 T. Maenam Khu A. Pluakdaeng Rayong 21140 Thailand | PHONE +66 0 3304 8555 | FAX +66 0 3304 8556
ALS LABORATORY GROUP (THAILAND) CO., LTD. An ALS Limited Company

Life Sciences

www.alsglobal.com

RIGHT SOLUTIONS RIGHT PARTNER



Analysis / Test Report

Client : Dow Chemical Thailand Ltd.
10 Moo 2, Asia Industrial Estate, Tambol Banchang, Amphur Banchang, Rayong Thailand
21130
P/O : 4516938822
Project Name : Water Testing
Project Location : AIE_PG Plant

Lot ID: 2549530

Date Received : Jun 04, 2025
Date Reported : Jun 12, 2025
Report Number : 3332393-2

Page 1 of 1

Sample Number	2549530-1
Sampled Date	Jun 04, 2025 10:30 AM
Sample Description	Wastewater
Location	PG Process
Date Analysis Commenced	Jun 05, 2025
Condition of Sample	Contained in two glass vials, three amber glass bottles and three plastic bottles, sample containers comply to pretreatment - preservation standards (APHA, USEPA)

Analyte	Unit	LOD	LOQ (LOR)	Result	Method	Testing Location
Water Testing						
Propylene Glycol	mg/L	-	1.0	12107	In-house method based on United States Environmental Protection Agency, EPA Method 8015 B	Bangkok
Total Organic Carbon	mg/L	0.01	0.1	8360	Standard Methods for the Examination of Water and Wastewater. APHA, AWWA & WEF, 24th ed., 2023, part 5310 B	Bangkok

Sampling By : Amonwich Wongsachai , Pattarapol Sawangjaitam

Remark :

- LOD : Limit of Detection
- "<" : Lower than LOQ (Limit of Quantitation) / LOR (Limit of Reporting)

Approved by

Suwimon C.

Suwimon Chairuangwut
Scientist (3)

Results apply to the sample(s) as submitted, unless the sampling was conducted by ALS. The report shall not be reproduced except in full without the written approval of the laboratory.

ภาคผนวก ค-5

ผลการตรวจวิเคราะห์คุณภาพน้ำทิ้งหลังผ่านการบำบัด
จากระบบบำบัดน้ำเสียส่วนกลาง



Analysis / Test Report

Client : Dow Chemical Thailand Ltd.
10 Moo 2, Asia Industrial Estate, Tambol Banchang, Amphur Banchang, Rayong Thailand
21130

P/O :
Project Name : Water Testing
Project Location : AIE_PG Plant

Lot ID: 24143086

Date Received : Jan 08, 2025
Date Reported : Jan 16, 2025
Report Number : 3215074-1

Page 1 of 1

Sample Number 24143086-2
Sampled Date Jan 08, 2025 2:00 PM
Sample Description Wastewater
Location Effluent PG
Date Analysis Commenced Jan 09, 2025
Condition of Sample Contained in one amber glass bottle. Sample containers comply to pretreatment - preservation standards (APHA / USEPA)

Analyte	Unit	LOD	LOQ (LOR)	Result	Method	Testing Location
Water Testing						
Propylene Glycol	mg/L	-	1.0	<1.0	In-house method based on United States Environmental Protection Agency, EPA Method 8015 B	Bangkok

Sampling By : Wanlop Hunchainaow , Pattarapol Sawangjaitam

Remark :

- LOD : Limit of Detection
- "<" : Lower than LOQ (Limit of Quantitation) / LOR (Limit of Reporting)

Approved by

Siriluk P.

Siriluk Bunnak
Section Head

Results apply to the sample(s) as submitted, unless the sampling was conducted by ALS. No part of this report may be reproduced in any form without written consent from the laboratory. ALS Laboratory Group (Thailand) strongly recommends that this report is not reproduced except in full.

ADDRESS 104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan, Khet Suan Luang, Bangkok 10250 Thailand | PHONE +66 0 2760 3000 | FAX +66 0 2760 3197
ALS LABORATORY GROUP (THAILAND) CO., LTD. An ALS Limited Company

Life Sciences

www.alsglobal.com

RIGHT SOLUTIONS RIGHT PARTNER



Analysis / Test Report

Client : Dow Chemical Thailand Ltd.
10 Moo 2, Asia Industrial Estate, Tambol Banchang, Amphur Banchang, Rayong Thailand
21130
P/O : 4516938822
Project Name : Water Testing
Project Location : AIE_PG Plant

Lot ID: 255322

Date Received : Feb 05, 2025
Date Reported : Feb 14, 2025
Report Number : 3234670-1

Page 1 of 1

Sample Number 255322-2
Sampled Date Feb 05, 2025 2:20 PM
Sample Description Wastewater
Location Effluent PG
Date Analysis Commenced Feb 06, 2025
Condition of Sample Contained in one amber glass bottle, sample containers comply to pretreatment - preservation standards (APHA, USEPA)

Analyte	Unit	LOD	LOQ (LOR)	Result	Method	Testing Location
Water Testing						
Propylene Glycol	mg/L	-	1.0	<1.0	In-house method based on United States Environmental Protection Agency, EPA Method 8015 B	Bangkok

Sampling By : Sansoen Khuiyoksui , Pattarapol Sawangjaitam

Remark :

- LOD : Limit of Detection
- "<" : Lower than LOQ (Limit of Quantitation) / LOR (Limit of Reporting)

Approved by

Siriluk P.

Siriluk Bunnak
Section Head

Results apply to the sample(s) as submitted, unless the sampling was conducted by ALS. The report shall not be reproduced except in full without the written approval of the laboratory.



Analysis / Test Report

Client : Dow Chemical Thailand Ltd.
10 Moo 2, Asia Industrial Estate, Tambol Banchang, Amphur Banchang, Rayong Thailand
21130
P/O : 4516938822
Project Name : Water Testing
Project Location : AIE_PG Plant

Lot ID: 2527496

Date Received : Apr 23, 2025
Date Reported : May 02, 2025
Report Number : 3294970-1

Page 1 of 1

Sample Number 2527496-2
Sampled Date Apr 23, 2025 11:30 AM
Sample Description Wastewater
Location Effluent PG
Date Analysis Commenced Apr 24, 2025
Condition of Sample Contained in one amber glass bottle, sample containers comply to pretreatment - preservation standards (APHA, USEPA)

Analyte	Unit	LOD	LOQ (LOR)	Result	Method	Testing Location
Water Testing						
Propylene Glycol	mg/L	-	1.0	<1.0	In-house method based on United States Environmental Protection Agency, EPA Method 8015 B	Bangkok

Sampling By : Sansoen Khuiyoksui

Remark :

- LOD : Limit of Detection
- "<" : Lower than LOQ (Limit of Quantitation) / LOR (Limit of Reporting)

Approved by

Siriluk P.

Siriluk Bunnak
Section Head

Results apply to the sample(s) as submitted, unless the sampling was conducted by ALS. The report shall not be reproduced except in full without the written approval of the laboratory.



Analysis / Test Report

Client : Dow Chemical Thailand Ltd.
10 Moo 2, Asia Industrial Estate, Tambol Banchang, Amphur Banchang, Rayong Thailand
21130
P/O : 4516938822
Project Name : Water Testing
Project Location : AIE_PG Plant

Lot ID: 2539224

Date Received : May 07, 2025
Date Reported : May 16, 2025
Report Number : 3307023-1

Page 1 of 1

Sample Number 2539224-2
Sampled Date May 07, 2025 11:45 AM
Sample Description Wastewater
Location Effluent PG
Date Analysis Commenced May 08, 2025
Condition of Sample Contained in one amber glass bottle, sample containers comply to pretreatment - preservation standards (APHA, USEPA)

Analyte	Unit	LOD	LOQ (LOR)	Result	Method	Testing Location
Water Testing						
Propylene Glycol	mg/L	-	1.0	<1.0	In-house method based on United States Environmental Protection Agency, EPA Method 8015 B	Bangkok

Sampling By : Surawit Narapong , Pattarapol Sawangjaitam

Remark :

- LOD : Limit of Detection
- "<" : Lower than LOQ (Limit of Quantitation) / LOR (Limit of Reporting)

Approved by

Suwimon C.

Suwimon Chairuangwut
Scientist (3)

Results apply to the sample(s) as submitted, unless the sampling was conducted by ALS. The report shall not be reproduced except in full without the written approval of the laboratory.



Analysis / Test Report

Client : Dow Chemical Thailand Ltd.
10 Moo 2, Asia Industrial Estate, Tambol Banchang, Amphur Banchang, Rayong Thailand
21130
P/O : 4516938822
Project Name : Water Testing
Project Location : AIE_PG Plant

Lot ID: 2549530

Date Received : Jun 04, 2025

Date Reported : Jun 12, 2025

Report Number : 3332394-1

Page 1 of 1

Sample Number 2549530-2
Sampled Date Jun 04, 2025 11:30 AM
Sample Description Wastewater
Location Effluent PG
Date Analysis Commenced Jun 05, 2025
Condition of Sample Contained in one amber glass bottle, sample containers comply to pretreatment - preservation standards (APHA, USEPA)

Analyte	Unit	LOD	LOQ (LOR)	Result	Method	Testing Location
Water Testing						
Propylene Glycol	mg/L	-	1.0	<1.0	In-house method based on United States Environmental Protection Agency, EPA Method 8015 B	Bangkok

Sampling By : Amonwich Wongsachai , Pattarapol Sawangjaitam

Remark :

- LOD : Limit of Detection
- "<" : Lower than LOQ (Limit of Quantitation) / LOR (Limit of Reporting)

Approved by

Suwimon C.

Suwimon Chairuangwut
Scientist (3)

Results apply to the sample(s) as submitted, unless the sampling was conducted by ALS. The report shall not be reproduced except in full without the written approval of the laboratory.

ภาคผนวก ค-6

ผลการตรวจวิเคราะห์คุณภาพน้ำหล่อเย็น



Analysis / Test Report

TESTING
No.0042

Client : Dow Chemical Thailand Ltd.
10 Moo 2, Asia Industrial Estate, Tambol Banchang, Amphur Banchang, Rayong Thailand 21130

P/O :
Project Name : 4 ater Testing
Project Location : AIE569 6lant

Lot ID: 24143086

Date Received : 8an 0W 202_
Date Reported : 8an 1G, 202_
Report - umber : 321_0J_v1

Page 1 of 1

Sample Number	2f 1f 30W3
Sampled Date	8an 0W 202_ 11:20 AM
Sample Description	Blowdown 4 ater
Location	69 Cooling Tower
Date Analysis Commenced	8an 0W 202_
Condition of Sample	Contained in two amber glass bottles and two plastic bottles. (ample containers comply to pretreatment v preserPatation standards H6UA / S(E6A)

Analyte	Unit	LOD	LOQ (LOR)	Result	Method	Testing Location
Water Testing						
COD	mg/L	1._	2._	3W	(tandard Methods for the Examination of 4 ater and 4 astewater. A6UA, A4 4 A & 4 EF, 2f th ed., 2023, part _220 D	Rayong
Oil & Grease	mg/L	v	3	7 3	(tandard Methods for the Examination of 4 ater and 4 astewater. A6UA, A4 4 A & 4 EF, 2f th ed., 2023, part _20 B	Rayong
pH at 2_ degree C		v	v	J._	(tandard Methods for the Examination of 4 ater and 4 astewater. A6UA, A4 4 A & 4 EF, 2f th ed., 2023, part f_00 v U HB)	Rayong
Total Dissolved (olids Dried at 1V0 degree C	mg/L	v	_	*f W	(tandard Methods for the Examination of 4 ater and 4 astewater. A6UA, A4 4 A & 4 EF, 2f th ed., 2023, part 2_f0 C	Rayong
Total (uspended (olids Dried at 103v10_ degree C	mg/L	v	_	G	(tandard Methods for the Examination of 4 ater and 4 astewater. A6UA, A4 4 A & 4 EF, 2f th ed., 2023, part 2_f0 D	Rayong

Sampling By : 4 anlop Uunchainaow ทะเบียนเลขที่ ว323จว003W, 6attarapol (awang-aitam ทะเบียนเลขที่ ว20f จว0002

Remark :
 - LOD : Limit of Detection
 - Q/Q : Lower than LOK (Limit of Quantitation) / LOR (Limit of Reporting)
 - Analyte(s) marked " " is/are not included in scope of Accreditation I (O/IEC 1102_
 - The laboratory has been accepted as an accredited laboratory complying with the I (O/IEC 1102_.

Technical Management

Photchanas.

Photchanas (eeda
(cientist H)
ทะเบียนเลขที่ ว323จว002W

Approved by

D. Chanchon.

De< Chanchon
(enior Manager
ทะเบียนเลขที่ ว323จว0001

Results apply to the sample(s) as submitted, unless the sampling was conducted by ALS. - o part of this report may be reproduced in any form without written consent from the laboratory.
ALS (Laboratory Group Thailand) strongly recommends that this report is not reproduced except in full.

ADDRESS 616/10 Moo 5 T. Maenam Khu A. Pluakdaeng Rayong 21140 Thailand | PHONE +66 0 3304 8555 | FAX +66 0 3304 8556
ALS LABORATORY GROUP (THAILAND) CO., LTD. An ALS Limited Company

Life Sciences

www.alsglobal.com

RIGHT SOLUTIONS RIGHT PARTNER



Analysis / Test Report

TESTING

No.0042

Client : Dow Chemical Thailand Ltd.

10 Moo 2, Asia Industrial Estate, Tambol Banchang, Amphur Banchang, Rayong Thailand
21130

P/O : 4516938822

Project Name : Water Testing

Project Location: AIE_PG Plant

Lot ID: 255322

Date Received : Feb 05, 2025

Date Reported : Feb 14, 2025

Report Number : 3234671-1

Page 1 of 1

Sample Number	255322-3
Sampled Date	Feb 05, 2025 10:55 AM
Sample Description	Blowdown Water
Location	PG Cooling Tower
Date Analysis Commenced	Feb 05, 2025
Condition of Sample	Contained in one amber glass bottle and two plastic bottles, sample containers comply to pretreatment - preservation standards (APHA, USEPA)

Analyte	Unit	LOD	LOQ (LOR)	Result	Guideline / Specification	Method	Testing Location
Water Testing							
COD	mg/L	1.5	25	58	≤120	Standard Methods for the Examination of Water and Wastewater. APHA, AWWA & WEF, 24th ed., 2023, part 5220 D	Rayong
Oil & Grease	mg/L	-	3	<3	≤5	Standard Methods for the Examination of Water and Wastewater. APHA, AWWA & WEF, 24th ed., 2023, part 5520 B	Rayong
pH at 25 degree C		-	-	7.8	5.5-9.0	Standard Methods for the Examination of Water and Wastewater. APHA, AWWA & WEF, 24th ed., 2023, part 4500 - H (B)	Rayong
Total Dissolved Solids Dried at 180 degree C	mg/L	-	5	910	≤3000	Standard Methods for the Examination of Water and Wastewater. APHA, AWWA & WEF, 24th ed., 2023, part 2540 C	Rayong
Total Suspended Solids Dried at 103-105 degree C	mg/L	-	5	9	≤50	Standard Methods for the Examination of Water and Wastewater. APHA, AWWA & WEF, 24th ed., 2023, part 2540 D	Rayong

Guideline : Effluent standard for factories, industrial estate and industrial park set by Notification of the Ministry of Natural Resource and Environment and effluent standard for factories and industrial park set by Notification of The Ministry of Industry dated June 07, B.E.2560 (2017).

Sampling By : Sansoen Khuiyoksui ทะเบียนเลขที่ ว-323-จ-0005 , Pattarapol Sawangjaitam ทะเบียนเลขที่ ว-204-จ-0002

Remark :

- LOD : Limit of Detection
- "<" : Lower than LOQ (Limit of Quantitation) / LOR (Limit of Reporting)
- Analyte(s) marked * is/are not included in scope of Accreditation ISO/IEC 17025.

Technical Management

Photchana S.

Photchana Seeda

Scientist (4)

ทะเบียนเลขที่ ว-323-จ-0028

Approved by

D. Changchon.

Dej Changchon

Senior Manager

ทะเบียนเลขที่ ว-323-ค-0001

Results apply to the sample(s) as submitted, unless the sampling was conducted by ALS. The report shall not be reproduced except in full without the written approval of the laboratory.

ADDRESS 616/10 Moo 5 T. Maenam Khu A. Pluakdaeng Rayong 21140 Thailand | PHONE +66 0 3304 8555 | FAX +66 0 3304 8556
ALS LABORATORY GROUP (THAILAND) CO., LTD. An ALS Limited Company

Life Sciences

www.alsglobal.com

RIGHT SOLUTIONS RIGHT PARTNER



Analysis / Test Report

TESTING

No.0042

Lot ID: 2527496

Date Received : Apr 23, 2025

Date Reported : Apr 30, 2025

Report Number : 32949v171

Client : Dow Chemical Thailand Ltd.

10 Moo 2, Asia Industrial Estate, Tambol Banchang, Amphur Banchang, Rayong Thailand 21130

P/O : 4516938822

Project Name : Water Testing

Project Location: AIE_PG Plant

Page 1 of 1

Sample Number	252v49673
Sampled Date	Apr 23, 2025 11:05 AM
Sample Description	Blowdown Water
Location	PG Cooling Tower
Date Analysis Commenced	Apr 23, 2025
Condition of Sample	Contained in one amber glass bottle and two plastic bottles, sample containers comply to pretreatment 7 preservation standards (AP(A, HUEPAS

Analyte	Unit	LOD	LOQ (LOR)	Result	Guideline / Specification	Method	Testing Location
Water Testing							
C) D	mg/L	1.5	25	50	≤120	Standard Methods for the Examination of Water and Wastewater. AP(A, AWWA x WE&, 24th ed., 2023, part 5220 D	Rayong
Oil & Grease	mg/L	7	3	<3	≤5	Standard Methods for the Examination of Water and Wastewater. AP(A, AWWA x WE&, 24th ed., 2023, part 5520 B	Rayong
pH at 25 degree C		7	7	v.v	5.5-9.0	Standard Methods for the Examination of Water and Wastewater. AP(A, AWWA x WE&, 24th ed., 2023, part 4500 7(fBS	Rayong
Total Dissolved Solids Dried at 180 degree C	mg/L	7	5	1180	≤3000	Standard Methods for the Examination of Water and Wastewater. AP(A, AWWA x WE&, 24th ed., 2023, part 2540 C	Rayong
Total Suspended Solids Dried at 103/105 degree C	mg/L	7	5	6	≤50	Standard Methods for the Examination of Water and Wastewater. AP(A, AWWA x WE&, 24th ed., 2023, part 2540 D	Rayong

Guideline : Effluent standard for factories, industrial estate and industrial park set by - notification of the Ministry of Natural Resource and Environment and effluent standard for factories and industrial park set by - notification of the Ministry of Industry dated June 0v, B.E.2560 f201vS

Sampling By : Uansoen Khuiyoksui ทะเบียนเลขที่ ๖๓๒๓๖๓๐๐๕

Remark :

- L) D : Limit of Detection
- Q<Q : Lower than L) j fLimit of QuantitationS/ L) R fLimit of ReportingS
- Analytes marked " is/are not included in scope of Accreditation IU) /IEC 1v025.
- Sampling is not included in scope of Accreditation IU) /IEC 1v025

Technical Management

Photchana S.

Photchana Ueada

Scientist f4S

ทะเบียนเลขที่ ๖๓๒๓๖๓๐๐๒๘

Approved by

D. Chumson.

De* Changchon

Senior Manager

ทะเบียนเลขที่ ๖๓๒๓๖๓๐๐๐๑

Results apply to the samples submitted, unless the sampling was conducted by ALS. The report shall not be reproduced except in full without the written approval of the laboratory.

ADDRESS 616/10 Moo 5 T. Maenam Khu A. Pluakdaeng Rayong 21140 Thailand | PHONE +66 0 3304 8555 | FAX +66 0 3304 8556
ALS LABORATORY GROUP (THAILAND) CO., LTD. An ALS Limited Company

Life Sciences

www.alsglobal.com

RIGHT SOLUTIONS RIGHT PARTNER



Analysis / Test Report

TESTING

No.0042

Lot ID: 2539224

Date Received : May 03, 2025

Date Reported : May 16, 2025

Report Number : 330J024-1

Client : Dow Chemical Thailand Ltd.

10 Moo 2, Asia Industrial Estate, Tambol Banchang, Amphur Banchang, Rayong Thailand 21130

P/O : 4516938822

Project Name : Water Testing

Project Location: AIE_PG Plant

Page 1 of 1

Sample Number	2539224-3
Sampled Date	May 03, 2025 11:25 AM
Sample Description	Blowdown Water
Location	PG Cooling Tower
Date Analysis Commenced	May 03, 2025
Condition of Sample	Contained in one amber glass bottle and two plastic bottles, sample containers comply to pretreatment - preservation standards (APHA, USEPA)

Analyte	Unit	LOD	LOQ (LOR)	Result	Guideline / Specification	Method	Testing Location
Water Testing							
COD	mg/L	1.5	25	13	≤120	Standard Methods for the Examination of Water and Wastewater. APHA, AWWA & WEF, 24th ed., 2023, part 5220 D	Rayong
Oil & Grease	mg/L	-	3	73	≤5	Standard Methods for the Examination of Water and Wastewater. APHA, AWWA & WEF, 24th ed., 2023, part 5520 B	Rayong
pH at 25 degree C		-	-	7.7	5.5-9.0	Standard Methods for the Examination of Water and Wastewater. APHA, AWWA & WEF, 24th ed., 2023, part 4500 - H (B)	Rayong
Total Dissolved Solids Dried at 180 degree C	mg/L	-	5	860	≤3000	Standard Methods for the Examination of Water and Wastewater. APHA, AWWA & WEF, 24th ed., 2023, part 2540 C	Rayong
Total Suspended Solids Dried at 103-105 degree C	mg/L	-	5	13	≤50	Standard Methods for the Examination of Water and Wastewater. APHA, AWWA & WEF, 24th ed., 2023, part 2540 D	Rayong

Guideline : Effluent standard for factories, industrial estate and industrial par* set by Notification of the Ministry of Natural Resource and Environment and effluent standard for factories and industrial par* set by Notification of The Ministry of Industry dated June 03, B.E.2560 (2017).

Sampling By : Surawit Narapong ทะเบียนเลขที่ ว-323-จ-0011 , Pattarapol Sawangjaitam ทะเบียนเลขที่ ว-204-จ-0002

Remark* :

- LOD : Limit of Detection
- Q/Q : Lower than LOK (Limit of quantitation) / LOR (Limit of Reporting)
- Analyte(s) marked " " is/are not included in scope of Accreditation ISO/IEC 17025.
- Sampling is not included in scope of accreditation ISO/IEC 17025

Technical Management

Photchana S.

Photchana Seeda

Scientist (4)

ทะเบียนเลขที่ ว-323-จ-0028

Approved by

D. Changchon.

Dej Changchon

Senior Manager

ทะเบียนเลขที่ ว-323-ค-0001

Results apply to the sample(s) as submitted, unless the sampling was conducted by ALS. The report shall not be reproduced except in full without the written approval of the laboratory.

ADDRESS 616/10 Moo 5 T. Maenam Khu A. Pluakdaeng Rayong 21140 Thailand | PHONE +66 0 3304 8555 | FAX +66 0 3304 8556
ALS LABORATORY GROUP (THAILAND) CO., LTD. An ALS Limited Company

Life Sciences

www.alsglobal.com

RIGHT SOLUTIONS RIGHT PARTNER



Analysis / Test Report

TESTING

No.0042

Lot ID: 2549530

Date Received : Jun 04, 2025

Date Reported : Jun 12, 2025

Report Number : 3332395-1

Client : Dow Chemical Thailand Ltd.

10 Moo 2, Asia Industrial Estate, Tambol Banchang, Amphur Banchang, Rayong Thailand 21130

P/O : 4516938822

Project Name : Water Testing

Project Location: AIE_PG Plant

Page 1 of 1

Sample Number	2549530-3
Sampled Date	Jun 04, 2025 10:25 AM
Sample Description	Blowdown Water
Location	PG Cooling Tower
Date Analysis Commenced	Jun 04, 2025
Condition of Sample	Contained in two amber glass bottles and two plastic bottles, sample containers comply to pretreatment - preservation standards (APHA, USEPA)

Analyte	Unit	LOD	LOQ (LOR)	Result	Guideline / Specification	Method	Testing Location
Water Testing							
COD	mg/L	1.5	25	45	≤120	Standard Methods for the Examination of Water and Wastewater. APHA, AWWA & WEF, 24th ed., 2023, part 5220 D	Rayong
Oil & Grease	mg/L	-	3	7.3	≤5	Standard Methods for the Examination of Water and Wastewater. APHA, AWWA & WEF, 24th ed., 2023, part 5520 B	Rayong
pH at 25 degree C		-	-	*.5	5.5-9.0	Standard Methods for the Examination of Water and Wastewater. APHA, AWWA & WEF, 24th ed., 2023, part 4500 - H (B)	Rayong
Total Dissolved Solids Dried at 180 degree C	mg/L	-	5	1020	≤3000	Standard Methods for the Examination of Water and Wastewater. APHA, AWWA & WEF, 24th ed., 2023, part 2540 C	Rayong
Total Suspended Solids Dried at 103-105 degree C	mg/L	-	5	7.5	≤50	Standard Methods for the Examination of Water and Wastewater. APHA, AWWA & WEF, 24th ed., 2023, part 2540 D	Rayong

Guideline : Effluent standard for factories, industrial estate and industrial park set by Notification of the Ministry of Natural Resource and Environment and effluent standard for factories and industrial park set by Notification of The Ministry of Industry dated June 0*, B.E.2560 (201*).

Sampling By : Amonwich Wongsachai ทะเบียนเลขที่ ว-323-จ-0040 , Pattarapol Sawangjaitam ทะเบียนเลขที่ ว-204-จ-0002

Remark:

- LOD : Limit of Detection
- Q/Q : Lower than LOK (Limit of quantitation) / LOR (Limit of Reporting)
- Analyte(s) marked " " is/are not included in scope of Accreditation ISO/IEC 17025.
- Sampling is not included in scope of accreditation ISO/IEC 17025

Technical Management

Photchana S.

Photchana Seeda

Scientist (4)

ทะเบียนเลขที่ ว-323-จ-0028

Approved by

D. Changchon.

Dej Changchon

Senior Manager

ทะเบียนเลขที่ ว-323-ค-0001

Results apply to the sample(s) as submitted, unless the sampling was conducted by ALS. The report shall not be reproduced except in full without the written approval of the laboratory.

ADDRESS 616/10 Moo 5 T. Maenam Khu A. Pluakdaeng Rayong 21140 Thailand | PHONE +66 0 3304 8555 | FAX +66 0 3304 8556
ALS LABORATORY GROUP (THAILAND) CO., LTD. An ALS Limited Company

Life Sciences

www.alsglobal.com

RIGHT SOLUTIONS RIGHT PARTNER

ภาคผนวก ค-7

ผลการตรวจวิเคราะห์คุณภาพน้ำใต้ดิน



Analysis / Test Report

Client : Dow Chemical Thailand Ltd.
10 Moo 2, Asia Industrial Estate, Tambol Banchang, Amphur Banchang, Rayong Thailand
21130
P/O : 4516938843
Project Name : Environmental Quality Monitoring
Project Location : AIEPGv Gant

Lot ID: 2517576

Date Received : Mar 21, 2025
Date Reported : Apr 02, 2025
Report Number : 324244972

Page 1 of 1

Sample Number 251f5f671
Sampled Date Mar 21, 2025 11:03 AM
Sample Description vroundwater
Location M(2
Date Analysis Commenced Mar 22, 2025
Condition of Sample Contained in one amber glass bottle and one plastic bottle, sample containers comply to pretreatment 7 preservation standards
HAGUA, S) EGAK

Analyte	Unit	LOD	LOQ (LOR)	Result	Method	Testing Location
Organic Compounds						
Gropylene oxide	mg/L	7	10	010	Inhouse method based on Snited) tates Environmental Protection Agency, EGA Method 8015 B	BangKoK

Sampling By : (anlop Uunchainaow ,) ansoen QhuiyoKsui

Remark :

- L" D : Limit oNDetection
- xOx : Lower than L" _ Hlimit oN_ uantitationk / L" R Hlimit oNReportingk

Approved by

Siriluk P.

)iriluk Bunnak
)ection Uead

Results apply to the sample as submitted, unless the sampling was conducted by ALS. The report shall not be reproduced except in full without the written approval of the laboratory.



Analysis / Test Report

Client : Dow Chemical Thailand Ltd.
10 Moo 2, Asia Industrial Estate, Tambol Banchang, Amphur Banchang, Rayong Thailand
21130
P/O : 4516938843
Project Name : Environmental Quality Monitoring
Project Location : AIE_PG Plant

Lot ID: 2517578

Date Received : Mar 21, 2025
Date Reported : Apr 02, 2025
Report Number : 3242459-2

Page 1 of 1

Sample Number	2517578-1
Sampled Date	Mar 21, 2025 11:20 AM
Sample Description	Groundwater
Location	MW 4
Date Analysis Commenced	Mar 22, 2025
Condition of Sample	Contained in one amber glass bottle and one plastic bottle, sample containers comply to pretreatment - preservation standards (APHA, USEPA)

Analyte	Unit	LOD	LOQ (LOR)	Result	Method	Testing Location
Organic Compounds						
Propylene oxide	mg/L	-	10	<10	In-house method based on United States Environmental Protection Agency, EPA Method 8015 B	Bangkok

Sampling By : Wanlop Hunchainaow , Pattarapol Sawangjaitam

Remark :

- LOD : Limit of Detection
- "<" : Lower than LOQ (Limit of Quantitation) / LOR (Limit of Reporting)

Approved by

Siriluk P.

Siriluk Bunnak
Section Head

Results apply to the sample(s) as submitted, unless the sampling was conducted by ALS. The report shall not be reproduced except in full without the written approval of the laboratory.



Analysis / Test Report

Client : Dow Chemical Thailand Ltd.
10 Moo 2, Asia Industrial Estate, Tambol Banchang, Amphur Banchang, Rayong Thailand
21130
P/O : 4516938843
Project Name : Environmental Quality Monitoring
Project Location : AIE_PG Plant

Lot ID: 2517579

Date Received : Mar 21, 2025
Date Reported : Apr 02, 2025
Report Number : 3242460-2

Page 1 of 1

Sample Number	2517579-1					
Sampled Date	Mar 21, 2025 11:35 AM					
Sample Description	Groundwater					
Location	MW 5					
Date Analysis Commenced	Mar 22, 2025					
Condition of Sample	Contained in one amber glass bottle and one plastic bottle, sample containers comply to pretreatment - preservation standards (APHA, USEPA)					
Analyte	Unit	LOD	LOQ (LOR)	Result	Method	Testing Location
Organic Compounds						
Propylene oxide	mg/L	-	10	<10	In-house method based on United States Environmental Protection Agency, EPA Method 8015 B	Bangkok

Sampling By : Wanlop Hunchainaow , Pattarapol Sawangjaitam

Remark :

- LOD : Limit of Detection
- "<" : Lower than LOQ (Limit of Quantitation) / LOR (Limit of Reporting)

Approved by

Siriluk P.

Siriluk Bunnak
Section Head

Results apply to the sample(s) as submitted, unless the sampling was conducted by ALS. The report shall not be reproduced except in full without the written approval of the laboratory.

ภาคผนวก ค-8

ผลการตรวจวิเคราะห์คุณภาพดิน



Analysis / Test Report

Client : Dow Chemical Thailand Ltd.

10 Moo 2, Asia Industrial Estate, Tambol Banchang, Amphur Banchang, Rayong Thailand
21130

P/O : 4515619934

Project Name : Environmental Quality Monitoring

Project Location : AIE_PG Plant

Lot ID: 2469000

Date Received : Jun 19, 2024

Date Reported : Jul 17, 2024

Report Number : 3038755-3

Page 1 of 1

Sample Number	2469000-1
Sampled Date	Jun 19, 2024 2:50 PM
Sample Description	Soil
Location	MW 2
Date Analysis Commenced	Jun 20, 2024
Condition of Sample	Packed in one plastic bag and one glass bottle, sample containers comply to pretreatment - preservation standards (APHA, USEPA)

Analyte	Unit	LOD	LOQ (LOR)	Result	Guideline / Specification	Method	Testing Location
Organic Compounds							
Propylene Oxide	mg/kg	-	20	<20	No Standard	In-house method based on United States Environmental Protection Agency, EPA Method 5035 and GC/FID	Bangkok

Guideline : Notification of the Ministry of Industry B.E. 2559 (2016) on Soil and Groundwater Contamination Criteria, Monitoring of Soil and Groundwater Quality, Report Submission and Report Preparation of Soil and Groundwater Quality, and Proposal Report of Soil and Groundwater Controlling and Reduction Measures

Note : This Analysis test report is reissued to supersede report No.3038755-2, Date Reported : Jun 27, 2024 due to revise analytical information.

Sampling By : Pattarapol Sawangjaitam

Remark :

- LOD : Limit of Detection
- "<" : Lower than LOQ (Limit of Quantitation) / LOR (Limit of Reporting)

Approved by

Nanthawadee Somboon
Specialist 2

Results apply to the sample(s) as submitted, unless the sampling was conducted by ALS. No part of this report may be reproduced in any form without written consent from the laboratory. ALS Laboratory Group (Thailand) strongly recommends that this report is not reproduced except in full.



Analysis / Test Report

Client : Dow Chemical Thailand Ltd.

10 Moo 2, Asia Industrial Estate, Tambol Banchang, Amphur Banchang, Rayong Thailand
21130

P/O : 4515619934

Project Name : Environmental Quality Monitoring

Project Location : AIE_PG Plant

Lot ID: 2469000

Date Received : Jun 19, 2024

Date Reported : Jul 17, 2024

Report Number : 3038756-3

Page 1 of 1

Sample Number	2469000-2
Sampled Date	Jun 19, 2024 11:30 AM
Sample Description	Soil
Location	MW 4
Date Analysis Commenced	Jun 20, 2024
Condition of Sample	Packed in one plastic bag and one glass bottle, sample containers comply to pretreatment - preservation standards (APHA, USEPA)

Analyte	Unit	LOD	LOQ (LOR)	Result	Guideline / Specification	Method	Testing Location
Organic Compounds							
Propylene Oxide	mg/kg	-	20	<20	No Standard	In-house method based on United States Environmental Protection Agency, EPA Method 5035 and GC/FID	Bangkok

Guideline : Notification of the Ministry of Industry B.E. 2559 (2016) on Soil and Groundwater Contamination Criteria, Monitoring of Soil and Groundwater Quality, Report Submission and Report Preparation of Soil and Groundwater Quality, and Proposal Report of Soil and Groundwater Controlling and Reduction Measures

Note : This Analysis test report is reissued to supersede report No.3038756-2, Date Reported : Jun 27, 2024 due to revise analytical information.

Sampling By : Pattarapol Sawangjaitam

Remark :

- LOD : Limit of Detection
- "<" : Lower than LOQ (Limit of Quantitation) / LOR (Limit of Reporting)

Approved by

Nanthawadee Somboon
Specialist 2

Results apply to the sample(s) as submitted, unless the sampling was conducted by ALS. No part of this report may be reproduced in any form without written consent from the laboratory. ALS Laboratory Group (Thailand) strongly recommends that this report is not reproduced except in full.



Analysis / Test Report

Client : Dow Chemical Thailand Ltd.

10 Moo 2, Asia Industrial Estate, Tambol Banchang, Amphur Banchang, Rayong Thailand
21130

P/O : 4515619934

Project Name : Environmental Quality Monitoring

Project Location : AIE_PG Plant

Lot ID: 2469000

Date Received : Jun 19, 2024

Date Reported : Jul 17, 2024

Report Number : 3038757-3

Page 1 of 1

Sample Number	2469000-3
Sampled Date	Jun 19, 2024 10:45 AM
Sample Description	Soil
Location	MW 5
Date Analysis Commenced	Jun 20, 2024
Condition of Sample	Packed in one plastic bag and one glass bottle, sample containers comply to pretreatment - preservation standards (APHA, USEPA)

Analyte	Unit	LOD	LOQ (LOR)	Result	Guideline / Specification	Method	Testing Location
Organic Compounds							
Propylene Oxide	mg/kg	-	20	<20	No Standard	In-house method based on United States Environmental Protection Agency, EPA Method 5035 and GC/FID	Bangkok

Guideline : Notification of the Ministry of Industry B.E. 2559 (2016) on Soil and Groundwater Contamination Criteria, Monitoring of Soil and Groundwater Quality, Report Submission and Report Preparation of Soil and Groundwater Quality, and Proposal Report of Soil and Groundwater Controlling and Reduction Measures

Note : This Analysis test report is reissued to supersede report No.3038757-2, Date Reported : Jun 27, 2024 due to revise analytical information.

Sampling By : Pattarapol Sawangjaitam

Remark :

- LOD : Limit of Detection
- "<" : Lower than LOQ (Limit of Quantitation) / LOR (Limit of Reporting)

Approved by

Nanthawadee Somboon
Specialist 2

Results apply to the sample(s) as submitted, unless the sampling was conducted by ALS. No part of this report may be reproduced in any form without written consent from the laboratory. ALS Laboratory Group (Thailand) strongly recommends that this report is not reproduced except in full.

ภาคผนวก ค-9

ผลการตรวจวัดความร้อนในสถานที่ปฏิบัติงาน



Analysis / Test Report

Client : Dow Chemical Thailand Ltd.

10 Moo 2, Asia Industrial Estate, Tambol Banchang, Amphur Banchang, Rayong
Thailand 21130

P/O : 4516938776

Project Name : Environmental Quality Monitoring

Project Location : AIE_PG Plant

Lot ID: 2529512

Date Received : Apr 24, 2025

Date Reported : Apr 28, 2025

Report Number: 3268547-1

Page 1 of 1

Sample Number 2529512-1
Parameter Heat Stress (Sampling Time : 09.00 AM - 11.00 AM)
Measurement Date Apr 24, 2025
Measurement by Natthapon Jiengwareewong
Location ปฏิบัติงาน 1 พื้นที่ (ชื่อ-นามสกุล ผู้ปฏิบัติงาน : - แผนก : -)

Location	Duration (min)	WBGT (°C)	NWB (°C)	GT (°C)	DB (°C)
บริเวณถังปฏิกิริยา	120	33.2	28.6	43.8	36.4
Average (WBGT)		33.2			
Guideline WBGT (°C)		34.0			

Reference Method : Wet Bulb Globe Temperature

Guideline:

- Notification of Department Labour Protection and Welfare on the Criteria and Procedures for Measurement and Analysis of Working Conditions in relation to Heat, Light or Noise Levels, including Duration and Types of Business that must perform (B.E. 2561)
- Ministerial Regulation on Prescribing of Standard for Administration and Management of Occupational Safety, Health and Environment in relation to Heat, Light and Noise, B.E.2559

Technical Management

Supot Salamteh
Section Head

Approved by

Wichan Choonharat
Assistant Manager

ADDRESS 616/10 Moo 5 T. Maenam Khu A. Pluakdaeng Rayong 21140 Thailand | PHONE +66 0 3304 8555 | FAX +66 0 3304 8556
ALS LABORATORY GROUP (THAILAND) CO., LTD. An ALS Limited Company

Life Sciences

www.alsglobal.com

RIGHT SOLUTIONS RIGHT PARTNER

ภาคผนวก ค-10

ผลการตรวจวัดระดับเสียงในสถานประกอบการ (Leq 12 hrs.)



Analysis / Test Report

Client : Dow Chemical Thailand Ltd.

10 Moo 2, Asia Industrial Estate, Tambol Banchang, Amphur Banchang, Rayong Thailand 21130

P/O : 4516938776

Project Name : Environmental Quality Monitoring

Project Location : AIE_PG Plant

Lot ID: 2518610

Date Received : Apr 25, 2025

Date Reported : Apr 30, 2025

Report Number: 3294636-1

Page 1 of 1

Sample Number 2518610-1
Parameter Noise (Leq 12 hrs.)
Location บริเวณพื้นที่ส่งปฏิกิริยา
Measurement Date Apr 24, 2025
Measurement by Natthapon Jiengwareewong

Time	Leq (dB(A))	Lmax (dB(A))	L90 (dB(A))
09:00 AM - 10:00 AM	74.7	83.9	74.4
10:00 AM - 11:00 AM	74.8	77.8	74.6
11:00 AM - 12:00 PM	74.7	76.7	74.5
12:00 PM - 01:00 PM	74.7	76.0	74.5
01:00 PM - 02:00 PM	74.8	77.0	74.5
02:00 PM - 03:00 PM	74.9	77.0	74.7
03:00 PM - 04:00 PM	75.2	89.2	74.8
04:00 PM - 05:00 PM	75.1	79.7	74.8
05:00 PM - 06:00 PM	75.1	80.4	74.9
06:00 PM - 07:00 PM	75.1	76.1	74.9
07:00 PM - 08:00 PM	75.1	76.0	74.9
08:00 PM - 09:00 PM	75.1	76.6	74.9
Leq Average 12 hrs. (dB(A))	74.9		
Lmax (dB(A))		89.2	
Standard (dB(A))	87	140	
Reference Method : ISO1996-1 and 1996-2			
Standard : ประกาศกระทรวงอุตสาหกรรม เรื่อง มาตรการคุ้มครองความปลอดภัย ในการประกอบกิจการโรงงานเกี่ยวกับสภาวะแวดล้อมในการทำงาน พ.ศ.๒๕๕๖			

Technical Management

Chontichak

Chonticha Subongkoch
Scientist (3)

dapproveA by

Supot S

Supot Salamteh
Section Head

ADDRESS 616/10 Moo 5 T. Maenam Khu A. Pluakdaeng Rayong 21140 Thailand | PHONE +66 0 3304 8555 | FAX +66 0 3304 8556
ALS LABORATORY GROUP (THAILAND) CO., LTD. An ALS Limited Company

Life Sciences

www.alsglobal.com

RIGHT SOLUTIONS RIGHT PARTNER



Analysis / Test Report

Client : Dow Chemical Thailand Ltd.

10 Moo 2, Asia Industrial Estate, Tambol Banchang, Amphur Banchang, Rayong Thailand 21130

P/O : 4516938776

Project Name : Environmental Quality Monitoring

Project Location : AIE_PG Plant

Lot ID: 2518610

Date Received : Apr 25, 2025

Date Reported : Apr 30, 2025

Report Number: 3294637-1

Page 1 of 1

Sample Number 2518610-2
Parameter Noise (Leq 12 hrs.)
Location บริเวณหอหล่อเย็น
Measurement Date Apr 24, 2025
Measurement by Natthapon Jiengwareewong

Time	Leq (dB(A))	Lmax (dB(A))	L90 (dB(A))
09:00 AM - 10:00 AM	82.3	85.8	82.1
10:00 AM - 11:00 AM	82.1	82.6	82.0
11:00 AM - 12:00 PM	82.1	82.7	82.0
12:00 PM - 01:00 PM	82.1	82.5	81.9
01:00 PM - 02:00 PM	82.3	83.0	82.0
02:00 PM - 03:00 PM	82.5	83.3	82.4
03:00 PM - 04:00 PM	82.6	83.2	82.5
04:00 PM - 05:00 PM	82.7	83.4	82.6
05:00 PM - 06:00 PM	82.8	83.3	82.7
06:00 PM - 07:00 PM	82.9	83.5	82.8
07:00 PM - 08:00 PM	82.9	83.4	82.8
08:00 PM - 09:00 PM	82.9	83.4	82.8

Leq Average 12 hrs. (dB(A))

82.5

Lmax (dB(A))

85.8

Standard (dB(A))

87

140

Reference Method : ISO1996-1 and 1996-2

Standard : ประกาศกระทรวงอุตสาหกรรม เรื่อง มาตรการคุ้มครองความปลอดภัย

ในการประกอบกิจการโรงงานเกี่ยวกับสภาวะแวดล้อมในการทำงาน พ.ศ.๒๕๔๖

Technical Management

Chontichak

Chonticha Subongkoch
Scientist (3)

dapproveA by

Supot S

Supot Salamteh
Section Head

ADDRESS 616/10 Moo 5 T. Maenam Khu A. Pluakdaeng Rayong 21140 Thailand | PHONE +66 0 3304 8555 | FAX +66 0 3304 8556
ALS LABORATORY GROUP (THAILAND) CO., LTD. An ALS Limited Company

Life Sciences

www.alsglobal.com

RIGHT SOLUTIONS RIGHT PARTNER

ภาคผนวก ค-11

ผลการตรวจวัดคุณภาพอากาศบริเวณการทำงาน
(แบบติดตัวบุคคล)



Analysis / Test Report

Report to : Dow Chemical Thailand Ltd.
10/4 Moo 2, Asia Industrial Estate, Tambol
Banchang, Amphur Banchang, Rayong
Thailand 21130
Attn : Komgrit Chaladtham
Phone : 0-3892-5614
Fax : -
Email : CKomgrit@dow.com

Project Name : Environmental Quality Monitoring

Lot ID: 203818

Location : AIE_PG Plant

Date Received : Jan 13, 2020

P/O :

Date Reported : Jan 17, 2020

Receipt No :

Report Number : 1561998-1

Cc. Email : PPChaiyadej@dow.com

Sampling by : Jaradrawee Sriuksa

Page 1 of 1

Reference Number 203818-1
Sampling Date Jan 13, 2020
Sample Description Air Quality
Location บริเวณพื้นที่ถังปฏิกิริยา
Personal Sampling คุณเกิดดิพงษ์ เพชรสังหนู
Condition of Sample Drawn into one sorbent tube, refrigerated
Date of Analysis Jan 14, 2020
Barometric Pressure 757 mmHg
Atmospheric Temperature 30.0 °C

Analyte	Sampling time	Result	Guideline Limit	Unit	Method	Guideline
Air Testing						
Propylene Oxide	09.30 AM - 11.30 AM	<0.10	100	ppm	NIOSH (1994), 1612	MOL

MOL : Announcement of the Department of Labour Protection and Welfare on Threshold Limit Values of Hazardous Chemical Substances Dated August 3, B.E. 2560 (2017)

The above results are valid only for the analyzed/tested sample(s) as indicated in this report. No part of this report or certificate may be reproduced in any form without written consent from the Laboratory. ALS Laboratory Group (Thailand) strongly recommends that this report is not reproduced except in full.

Approved by

Sararat Mongkonjirawut
Scientist (4)

ภาคผนวก ง

เอกสารสอบเทียบเครื่องมือที่ใช้ในการวิเคราะห์



right solutions.
right partner.

รายการเครื่องมือที่ใช้ในการวิเคราะห์ / ทดสอบ

Sample Name	Parameter	Equipment Name	ID No.	Calibrated Date	Next Cal	Freq. Calibrate (Months)
Ambient	Propylene Oxide	DRYCAL FLOWMETER	RYG_FS0208	13-Feb-24	13-Aug-25	18
Ambient	Propylene Oxide	DRYCAL FLOWMETER	BKK_FS0614	21-May-24	21-May-25	12
Ambient	Propylene Oxide	DRYCAL FLOWMETER	RYG_FS0208	27-Jan-25	26-Jan-26	12
Ambient	Propylene Oxide	DRYCAL FLOWMETER	BKK_FS0614	9-Sep-24	9-Sep-25	12
Ambient	Propylene Oxide	Air Sampling Pump	RYG_FS0106	6-Jan-25	6-Apr-25	3
Ambient	Propylene Oxide	Air Sampling Pump	RYG_FS0108	6-Jan-25	6-Apr-25	3
Ambient	Propylene Oxide	Air Sampling Pump	RYG_FS0128	7-Apr-25	7-Jul-25	3
Ambient	Propylene Oxide	Air Sampling Pump	RYG_FS0108	6-Apr-25	6-Jul-25	3
Ambient	Propylene Oxide	Air Sampling Pump	RYG_FS0368	6-Apr-25	6-Jul-25	3
Ambient	Propylene Oxide	GC-FID	BKK_EN0126	22-Oct-24	22-Apr-26	18
Noise	Leq 24 hrs	Sound Calibrator	RYG_FS0496	19-Mar-25	19-Mar-26	12
Noise	Leq 24 hrs	Sound Level Meter	RYG_FS0492	27-Jan-25	26-Jan-26	12
Noise	Leq 24 hrs	Sound Level Meter	RYG_FS0389	27-Jan-25	26-Jan-26	12
Noise	Leq 24 hrs	Sound Level Meter	RYG_FS0388	19-Mar-25	19-Mar-26	12
Noise	Leq 12 hrs	Sound Calibrator	RYG_FS0213	16-Jan-25	16-Jan-26	12
Noise	Leq 12 hrs	Sound Level Meter	RYG_FS0621	27-Jan-25	26-Jan-26	12
Noise	Leq 12 hrs	Sound Level Meter	RYG_FS0432	27-Jan-25	26-Jan-26	12
Heat	Heat Stress	Heat Stress Monitor	RYG_FS0236	17-May-24	17-May-25	12
Rayong Lab	pH at 25 °C	pH meter	RYG_EN0183	19-Jan-24	19-Jul-25	18
Rayong Lab	BOD	DO meter with Sensor	RYG_EN0032	20-Jan-25	20-Jul-26	18
Rayong Lab	BOD	Incubator	RYG_EN0154	1-Nov-24	1-May-26	18
Rayong Lab	BOD	Burette	RYG_EN0216	24-Sep-24	24-Sep-25	12
Rayong Lab	COD	Spectrophotometer	RYG_EN0037	18-Mar-25	18-Sep-26	18
Rayong Lab	Total Suspended Solids	Electronic Balance	RYG_EN0002	20-Feb-25	20-Feb-26	12
Rayong Lab	Total Suspended Solids	Hot Air Oven	RYG_EN0010	21-Mar-24	21-Sep-25	18
Rayong Lab	Oil & Grease	Electronic Balance	RYG_EN0002	20-Feb-25	20-Feb-26	12
Rayong Lab	Oil & Grease	Hot Air Oven	RYG_EN0213	19-Mar-25	19-Mar-26	12
Rayong Lab	Oil & Grease	Water Bath	RYG_EN0061	21-Mar-24	21-Sep-25	18
Water Lab	Propylene Glycol	Gas Chromatography (FID)	BKK_EN0126	22-Oct-24	22-Apr-26	18
Water Lab	Total Organic carbon	TOC Analyzer	BKK_EN0066	26-Jun-24	26-Jun-25	12
Water Lab	Propylene Oxide	Gas Chromatography (FID)	BKK_EN0126	22-Oct-24	22-Apr-26	18
Soil	Propylene Oxide	Gas Chromatography (FID)	BKK_EN0126	21-Apr-23	21-Oct-24	12

Certificate of Calibration

Customer

Name : ALS Laboratory Group Thailand Co., Ltd.
Address : 104 Soi Phatthanakan 40, Phatthanakan Road, Suan Luang, Bangkok
10250

Certificate No : 24-AFM-033

Request No : Req-2024-0241

Unit Under Calibration Details

Measurement Item : Primary Flow Calibrator
Manufacturer : Bios
Model : Defender 510-L
Serial Number : 130027
ID : RYG_FS0208
Location of Calibration : LAB 4 AIR VELOCITY METER

Sensor Model : -

Sensor Serial Number : -

Calibration Environment and Details

Temperature : 23 °C ± 3 °C
Humidity : 55 %RH ± 20 %RH
Barometric Pressure : 1013 hPa ± 10 hPa
Received Date : 31 January 2024
Calibration Date : 13 February 2024



Calibration Procedure : In-house method CP-AFM-01 by Comparison technique with Standard Primary Flow Calibrator

Reference Standard	Model	Serial Number	Traceble	Due Calibration
Air Flow Meter	Gilibrator 3 Low flow	18501010006	Sensidyne	12 July 2024
Air Flow Meter	Gilibrator 3 Standard flow	19031011003	Sensidyne	12 July 2024
Temperature meter	GT 11	08000057	Qreborn	27 February 2024
Pressure meter	CPG2400	41000KDU/651882	TPA	9 November 2024

Traceability :

This Certificate is traceable to SI Unit through Sensidyne A2LA Accreditation No. 3943.01

Note :

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor $k = 2$, providing a level of confidence approximately 95 %.

Calibration By : *me*
Mr. Noppadon Luangart
Service Calibration Engineer

Approved By : *pacit*
Mr. Pacit Mathavorn
Calibration Engineer Supervisor

Issue Date : 13 February 2024

Certificate No : 24-AFM-033

Request No : Req-2024-0241

Result of Calibration : Without Adjustment

Temperature (°C)	Pressure (kPa)	STD (cc/min)	UUC (cc/min)	Error (cc/min)	Uncertainty (cc/min)
24.50	101.26	20	19.965	0.0	1.3
24.20	101.25	101	100.50	-0.5	2.8
24.00	101.31	200	199.13	-0.9	5.6
23.90	101.42	301	303.56	2.6	8.4
24.10	101.41	401	404.57	4	11
24.10	101.49	480	483.81	3.8	7.0

Note

STD : Standard

UUC : Unit Under Calibration

- UUC Reference Condition : At atmospheric pressure and room temperature condition

- Flow Rate was corrected for non-standard operating condition by using equation :

$$Q_{meas} = Q_{ref} \times \frac{P_{ref}}{P_{meas}} \times \frac{T_{meas}}{T_{ref}}$$

where Q = Flow Rate

P = Absolute Pressure

T = Absolute Temperature

Meas = Measurement Condition

ref = Standard Condition

* Indicates non accredited

End of Certificate



Calibration Certificate

Certificate No. 610563
Product 200-510M Defender 510 Medium Flow
Serial No. 151114
Cal. Date 21-May-2024

Sold To:

All calibrations are performed in accordance with ISO 17025 at Mesa Laboratories, Inc., 12100 W. 6th Ave, Lakewood, CO 80228, an ISO 17025:2017 accredited laboratory through NVLAP. This report shall not be reproduced except in full without the written approval of the laboratory. Results only relate to the items calibrated. This report must not be used to claim product certification, approval, or endorsement by NVLAP, NIST, or any agency of the U.S. Government.

As Received Calibration Data

Technician	Derek Dellape	Lab. Pressure		614.2 mmHg
		Lab. Temperature		24.3 °C
Instrument Reading	Lab Standard Reading	Deviation	Allowable Deviation	As Received
0 ccm	4504.81 ccm	-100.0%	1.00%	Out of Tolerance
0 ccm	1000.98 ccm	-100.0%	1.00%	Out of Tolerance
0 ccm	249.55 ccm	-100.0%	1.00%	Out of Tolerance

Mesa Laboratories Standards Used

Description	Standard Serial Number	Calibration Date	Calibration Due Date
ML-800-24	117991	13-Nov-2023	13-Nov-2024

REVIEW BY Narakom P.

APPROVED BY [Signature]

NEXT CAL. DATE 21/5/25

As Shipped Calibration Data

Certificate No	610563	Lab. Pressure	617 mmHg
Technician	Derek Dellape	Lab. Temperature	24.6 °C

Instrument Reading	Lab Standard Reading	Deviation	Allowable Deviation	As Shipped
4482.47 ccm	4493.49 ccm	-0.25%	1.00%	In Tolerance
997.25 ccm	996.83 ccm	0.04%	1.00%	In Tolerance
248.51 ccm	248.67 ccm	-0.06%	1.00%	In Tolerance

Mesa Laboratories Standards Used

Description	Standard Serial Number	Calibration Date	Calibration Due Date
ML-800-24	211063	04-Oct-2023	04-Oct-2024

Calibration Notes

The expanded uncertainty of flow has a coverage factor of $k = 2$ for a confidence interval of approximately 95%.

Flow testing is in accordance with our test number MP-00672 with an expanded uncertainty of 0.27% using high-purity nitrogen or filtered laboratory air.

Traceability to the International System of Units (SI) is verified by accreditation to ISO/IEC 17025 by NVLAP under NVLAP Code 200661-0.

Technician Notes:

By:

Approved By:



Derek Dellape
Production Assembler II



Troy Thacker
Quality Engineer

Mesa Laboratories, Inc. certifies that the above instrument meets or exceeds published specifications, and that the calibration results in this certificate were obtained using equipment capable of producing results that are traceable through NIST to the International System of Units (SI). Calibration results are in compliance with ISO/IEC 17025:2017. Calibrations process has a Test Uncertainty Ratio (TUR) of 4:1 or greater. Any Pass/Fail determination is made without taking measurement uncertainty into account and is based on UUT performance against required tolerance only.

Certificate of Calibration

Customer

Name : ALS Laboratory Group Thailand Co., Ltd.
Address : 104 Soi Phatthanakan 40, Phatthanakan Road, Suan Luang,
Bangkok 10250

Certificate No : 25-AFM-023

Request No : Req-2025-0169

Unit Under Calibration Details

Measurement Item : Air Flow Meter
Manufacturer : Mesa Labs
Model : 200-510L
Serial Number : 130027
ID : RYG_FS0208

Accuracy : 1% of Reading

Sensor Model : -

Sensor Serial Number : -

Instrument Status : Used

Location of Calibration : LAB 4 AIR VELOCITY METER

Calibration Environment and Details

Temperature : 23 °C ± 3 °C
Humidity : 55 %RH ± 20 %RH
Barometric Pressure : 1013 hPa ± 10 hPa
Received Date : 21 January 2025
Calibration Date : 27 January 2025

Calibration Procedure : In-house method CP-AFM-01 by Comparison technique with Standard Primary Flow Calibrator

REVIEW BY 
APPROVED BY 
NEXT CAL DATE.....26/01/26.....


Reference Standard	Model	Serial Number	Traceble	Due Calibration
Air Flow Meter	Gilibrator 3 Low flow	18501010006	Sensidyne	6 August 2025
Air Flow Meter	Gilibrator 3 Standard flow	19031011003	Sensidyne	2 August 2025
Temperature meter	GT 11	08000057	Qreborn	1 March 2025
Pressure meter	CPG2400	41000KDU/651882	TPA	21 October 2025


Traceability :

This Certificate is traceable to SI Unit through Sensidyne A2LA Accreditation No. 3943.01

Note :

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor $k = 2$, providing a level of confidence approximately 95 %.

Calibration By : 
Mr. Noppadon Luangart
Service Calibration Engineer

Approved By : 
Mr. Pacit Mathavorn
Calibration Engineer Supervisor

Issue Date : 27 January 2025

Certificate No : 25-AFM-023

Request No : Req-2025-0169

Result of Calibration : Without Adjustment

Temperature (°C)	Pressure (kPa)	STD (cc/min)	UUC (cc/min)	Error (cc/min)	Uncertainty (cc/min)	MPE (cc/min)	Result
22.50	100.90	20	19.854	-0.1	1.3	0.2	Pass1
22.50	100.90	50	49.732	-0.3	3.3	0.5	Pass1
22.60	100.90	101	100.77	-0.2	2.8	1.0	Pass1
22.70	100.90	151	150.23	-0.8	4.2	1.5	Pass1
22.70	100.90	201	200.39	-0.6	5.6	2.0	Pass1
22.70	100.90	301	300.69	-0.3	8.4	3.0	Pass1
22.80	100.90	400	402.96	3.0	11	4.0	Pass1
23.10	100.90	500	504.62	4.6	7.2	5.0	Pass1

Note

STD : Standard UUC : Unit Under Calibration

- UUC Reference Condition : At atmospheric pressure and room temperature condition
- Flow Rate was corrected for non-standard operating condition by using equation :

$$Q_{\text{meas}} = Q_{\text{ref}} \times \frac{P_{\text{ref}}}{P_{\text{meas}}} \times \frac{T_{\text{meas}}}{T_{\text{ref}}}$$

where Q = Flow Rate P = Absolute Pressure T = Absolute Temperature
 Meas = Measurement Condition ref = Standard Condition

* Indicates non accredited

MPE = Maximum Permissible Error (Specified in Manufacturer's Specifications)

N/A = Not Available, Customer does not require a statement of conformity.

Certificate No : 25-AFM-023

Request No : Req-2025-0169

Decision Rule for Statements of Conformity


The standard decision rule employed for the statements of conformity to each calibration result will be applied using ILAC-G8:09/2019; Guidelines on the Reporting of Compliance with Specification as following Fig. and statements

Pass = The measurement result plus the expanded uncertainty with a 95% coverage probability were within the limit.

Pass¹ = The measurement result was within the limit. However, a portion of the expanded uncertainty of measurement at 95% exceeds the limit.

Fail¹ = The measurement result was out of the limit. However, a portion of the expanded uncertainty of measurement at 95% is within the limit.

Fail = The measurement result plus the expanded uncertainty with a 95% coverage probability were outside the limit.

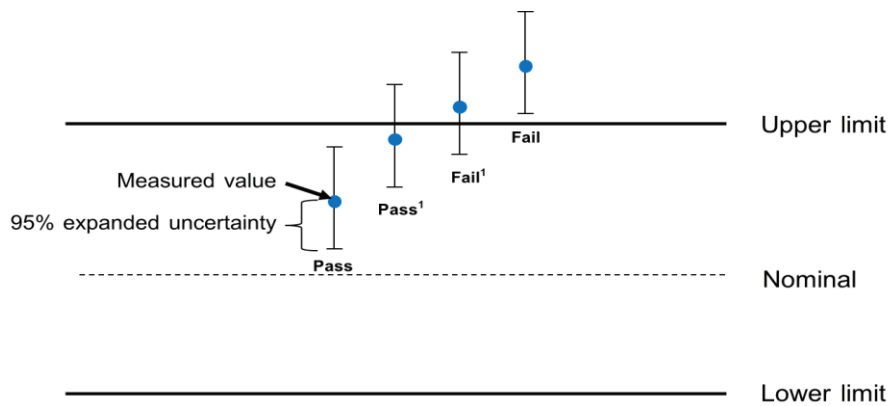

End of Certificate

Certificate of Calibration

Customer

Name : ALS Laboratory Group Thailand Co., Ltd.
Address : 104 Soi Phatthanakan 40, Phatthanakan Road, Suan Luang,
Bangkok 10250

Certificate No : 24-AFM-179

Request No : Req-2024-1987

Unit Under Calibration Details

Measurement Item : Air Flow Meter
Manufacturer : MesaLabs Accuracy : 1% of Reading
Model : Defender 510-M Sensor Model : -
Serial Number : 151114 Sensor Serial Number : -
ID : BKK_FS0614 Instrument Status : Used
Location of Calibration : LAB 4 AIR VELOCITY METER

Calibration Environment and Details

Temperature : 23 °C ± 3 °C
Humidity : 55 %RH ± 20 %RH
Barometric Pressure : 1013 hPa ± 10 hPa
Received Date : 30 August 2024
Calibration Date : 9 September 2024
Calibration Procedure : In-house method CP-AFM-01 by Comparison technique with Standard Primary Flow Calibrator



Reference Standard	Model	Serial Number	Traceable	Due Calibration
Air Flow Meter	Gilibrator 3 Low flow	18501010006	Sensidyne	6 August 2025
Air Flow Meter	Gilibrator 3 Standard flow	19031011003	Sensidyne	2 August 2025
Temperature meter	GT 11	08000057	Qreborn	1 March 2025
Pressure meter	CPG2400	41000KDU/651882	TPA	9 November 2024

Traceability :

This Certificate is traceable to SI Unit through Sensidyne A2LA Accreditation No. 3943.01

Note :

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor $k = 2$, providing a level of confidence approximately 95 %.

Calibration By : [Signature]
Mr. Noppadon Luangart
Service Calibration Engineer

Approved By : [Signature]
Mr. Pacit Mathavorn
Calibration Engineer Supervisor

Issue Date : 9 September 2024

Certificate No : 24-AFM-179

Request No : Req-2024-1987

Result of Calibration : Without Adjustment

Temperature (°C)	Pressure (kPa)	STD (cc/min)	UUC (cc/min)	Error (cc/min)	Uncertainty (cc/min)	MPE (cc/min)	Result
24.70	100.95	100	100.41	0.4	2.8	1.0	N/A
24.90	100.90	502	500.47	-1.5	7.1	5.0	N/A
24.90	100.97	1003	1001.3	-2	14	10.0	N/A
25.00	100.92	2014	2009.9	-4	29	20.1	N/A
25.20	101.03	3043	3058.3	15	44	30.4	N/A
25.30	101.10	4043	4005.1	-38	57	40.4	N/A
25.50	101.15	5052	5003.9	-48	74	50.5	N/A

Note

STD : Standard UUC : Unit Under Calibration

- UUC Reference Condition : At atmospheric pressure and room temperature condition

- Flow Rate was corrected for non-standard operating condition by using equation :

$$Q_{meas} = Q_{ref} \times \frac{P_{ref}}{P_{meas}} \times \frac{T_{meas}}{T_{ref}}$$

where Q = Flow Rate P = Absolute Pressure T = Absolute Temperature

Meas = Measurement Condition ref = Standard Condition

* Indicates non accredited

MPE = Maximum Permissible Error (Specified in Manufacturer's Specifications)

N/A = Not Available, Customer does not require a statement of conformity.

Certificate No : 24-AFM-179

Request No : Req-2024-1987

Decision Rule for Statements of Conformity


The standard decision rule employed for the statements of conformity to each calibration result will be applied using ILAC-G8:09/2019; Guidelines on the Reporting of Compliance with Specification as following Fig. and statements

Pass = The measurement result plus the expanded uncertainty with a 95% coverage probability were within the limit.

Pass¹ = The measurement result was within the limit. However, a portion of the expanded uncertainty of measurement at 95% exceeds the limit.

Fail¹ = The measurement result was out of the limit. However, a portion of the expanded uncertainty of measurement at 95% is within the limit.

Fail = The measurement result plus the expanded uncertainty with a 95% coverage probability were outside the limit.

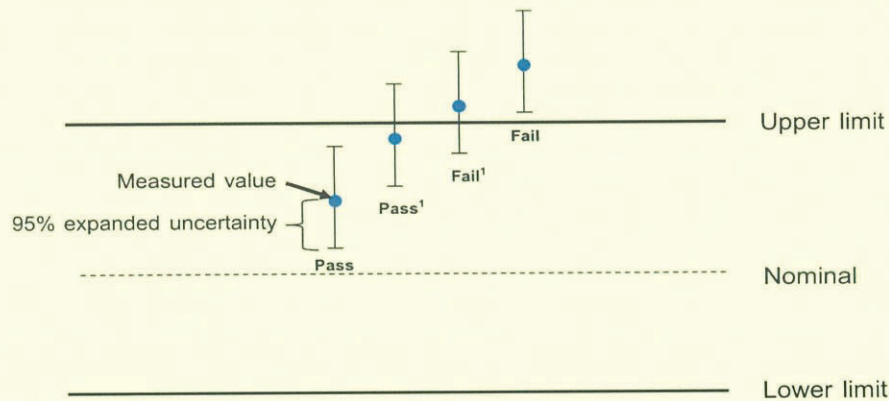

End of Certificate



Air Sampling Pump Calibration Report

Air Sampling Pump Detail

Calibration Date	: 6 Jan 2025	Next cal.	: 6 Apr 2025
Air Sampling Pump ID	: RYG_FS0106	Barometric (mmHg)	: 755.9
Serial No.	: 20220731509	Temperature (°C)	: 25.9

Reference Standard Low Flow Meter

Brand	: MesaLabs	ID	: RYG_FS0208
Model	: Defender 510-L	Serial No.	: 130027
Due Date	: 13-Aug-25		

Reference Standard High Flow Meter

Brand	: MesaLabs	ID	: BKK_FS0614
Model	: Defender 510-M	Serial No.	: 151114
Due Date	: 21-May-25		

Calibration Data

Air Sampling Pump setting (cc/min)	Reference Standard Flow Reading (cc/min)			Avg. (cc/min)	Acceptable (cc/min)		Evaluation Pass/ Fail
	1	2	3				
20	20.5	20.5	20.4	20.5	21	19	Passed
50	50.1	50.0	49.9	50.0	52.5	47.5	Passed
100	100.1	100.2	100.1	100.1	105	95	Passed
200	200.0	200.7	200.6	200.4	210	190	Passed
500	497.6	499.1	498.2	498.3	515	485	Passed
1000	995.0	996.4	998.8	996.7	1010	990	Passed
2000	1992.2	1990.3	2008.0	1996.8	2020	1980	Passed
2500	2517.0	2502.2	2503.2	2507.5	2550	2450	Passed

Note : Reference Specifications $\pm 5\%$ of set flow or $\pm 3\%$ cc/min whichever is Higher

Calibrated by : 

(Mr. Nantawat Sarin)
Enviro Field Services Scientist (1)

Approved By : 

(Mr. Wichan Choonharat)
Enviro Field Services Manager

**Air Sampling Pump Calibration Report****Air Sampling Pump Detail**

Calibration Date	: 6 Jan 2025	Next cal.	: 6 Apr 2025
Air Sampling Pump ID	: RYG_FS0108	Barometric (mmHg)	: 755.9
Serial No.	: 20150310157	Temperature (°C)	: 25.9

Reference Standard Low Flow Meter

Brand	: MesaLabs	ID	: RYG_FS0208
Model	: Defender 510-L	Serial No.	: 130027
Due Date	: 13-Aug-25		

Reference Standard High Flow Meter

Brand	: MesaLabs	ID	: BKK_FS0614
Model	: Defender 510-M	Serial No.	: 151114
Due Date	: 21-May-25		

Calibration Data

Air Sampling Pump setting (cc/min)	Reference Standard Flow Reading (cc/min)			Avg. (cc/min)	Acceptable (cc/min)		Evaluation Pass/ Fail
	1	2	3				
20	19.8	20.7	20.2	20.2	21	19	Passed
50	50.6	50.7	50.7	50.7	52.5	47.5	Passed
100	98.7	99.7	100.2	99.5	105	95	Passed
200	197.5	197.0	197.6	197.4	210	190	Passed
500	512.7	489.7	500.4	500.9	515	485	Passed
1000	1002.9	1001.2	998.7	1000.9	1010	990	Passed
2000	2015.6	1996.1	1995.5	2002.4	2020	1980	Passed
2500	2503.2	2514.9	2517.6	2511.9	2550	2450	Passed

Note : Reference Specifications $\pm 5\%$ of set flow or $\pm 3\%$ cc/min whichever is Higher

Calibrated by :

(Mr. Nantawat Sarin)
Enviro Field Services Scientist (1)

Approved By :

(Mr. Wichan Choonharat)
Enviro Field Services Manager



Certificate of Calibration

Certificate No. C-070425-RYG_FS0128

Air Sampling Pump Detail

Equipment name : Personal Air Sampling Pump
Brand : Gilian
Model/Type : GilAir Plus

Equipment ID : RYG_FS0128
Serial No. : 20150410004
Calibration Date : 07-Apr-25
Next calibration date : 07-Jul-25

Reference Standard Low Flow Meter

Equipment name : Air Flow Meter
Brand : MesaLabs
Model/Type : Defender 510-L

Equipment ID : RYG_FS0208
Serial No. : 130027
Calibration Date : 27-Jan-25
Due Date : 26-Jan-26

Reference Standard High Flow Meter

Equipment name : Air Flow Meter
Brand : MesaLabs
Model/Type : Defender 510-M

Equipment ID : BKK_FS0614
Serial No. : 151114
Calibration Date : 9-Sep-24
Due Date : 9-Sep-25

Calibration Data

Air Sampling Pump setting (cc/min)	Reference Std. Flow Reading (cc/min)			Avg. (cc/min)	%Error acceptance	Acceptable range (cc/min)			Evaluation (Pass/ Fail)
	1	2	3						
Low Flow									
20	19.8	20.3	20.6	20.2	5%	19	-	21	Passed
50	49.3	49.3	49.4	49.3	5%	48	-	53	Passed
100	99.3	99.4	99.4	99.4	5%	95	-	105	Passed
200	199.4	197.4	198.5	198.4	5%	190	-	210	Passed
High Flow									
500	506.7	504.1	508.0	506.3	3%	485	-	515	Passed
1000	1015.2	1010.4	1012.4	1012.7	3%	970	-	1030	Passed
2000	1992.6	1998.1	1996.3	1995.7	3%	1940	-	2060	Passed
2500	2492.3	2494.4	2490.5	2492.4	3%	2425	-	2575	Passed
4000	3998.7	4001.2	3999.9	3999.9	3%	3880	-	4120	Passed

----- END OF REPORT -----

Calibrated By: นันทพล

(Mr.Natchapon Thamklang)

RYG Field Services Scientist (1)

Issue date : 07-Apr-25

Approved By: Supot S

(Mr.Supot Salamteh)

RYG Field Services Section Head



Certificate of Calibration

Certificate No. C-060425-RYG_FS0108

Air Sampling Pump Detail

Equipment name : Personal Air Sampling Pump
Brand : Gilian
Model/Type : GilAir PlusEquipment ID : RYG_FS0108
Serial No. : 20150310157
Calibration Date : 06-Apr-25
Next calibration date : 06-Jul-25

Reference Standard Low Flow Meter

Equipment name : Air Flow Meter
Brand : MesaLabs
Model/Type : Defender 510-LEquipment ID : RYG_FS0208
Serial No. : 130027
Calibration Date : 27-Jan-25
Due Date : 26-Jan-26

Reference Standard High Flow Meter

Equipment name : Air Flow Meter
Brand : MesaLabs
Model/Type : Defender 510-MEquipment ID : BKK_FS0614
Serial No. : 151114
Calibration Date : 9-Sep-24
Due Date : 9-Sep-25

Calibration Data

Air Sampling Pump setting (cc/min)	Reference Std. Flow Reading (cc/min)			Avg. (cc/min)	%Error acceptance	Acceptable range (cc/min)	Evaluation (Pass/ Fail)
	1	2	3				
Low Flow							
20	20.5	19.7	20.4	20.2	5%	19 - 21	Passed
50	50.1	49.7	51.2	50.3	5%	48 - 53	Passed
100	101.1	100.3	101.5	101.0	5%	95 - 105	Passed
200	201.8	204.4	202.3	202.8	5%	190 - 210	Passed
High Flow							
500	503.8	507.4	510.4	507.2	3%	485 - 515	Passed
1000	994.7	991.4	996.2	994.1	3%	970 - 1030	Passed
2000	2000.7	2019.4	2006.3	2008.8	3%	1940 - 2060	Passed
2500	2516.4	2518.4	2517.5	2517.4	3%	2425 - 2575	Passed

----- END OF REPORT -----

Calibrated By: นันทพล

(Mr.Natchapon Thamklang)

RYG Field Services Scientist (1)

Issue date : 06-Apr-25

Approved By: Supot S

(Mr.Supot Salamteh)

RYG Field Services Section Head



Certificate of Calibration

Certificate No. C-060425-RYG_FS0368

Air Sampling Pump Detail

Equipment name : Personal Air Sampling Pump
Brand : Gilian
Model/Type : GilAir Plus

Equipment ID : RYG_FS0368
Serial No. : 20180610061
Calibration Date : 06-Apr-25
Next calibration date : 06-Jul-25

Reference Standard Low Flow Meter

Equipment name : Air Flow Meter
Brand : MesaLabs
Model/Type : Defender 510-L

Equipment ID : RYG_FS0208
Serial No. : 130027
Calibration Date : 27-Jan-25
Due Date : 26-Jan-26

Reference Standard High Flow Meter

Equipment name : Air Flow Meter
Brand : MesaLabs
Model/Type : Defender 510-M

Equipment ID : BKK_FS0614
Serial No. : 151114
Calibration Date : 9-Sep-24
Due Date : 9-Sep-25

Calibration Data

Air Sampling Pump setting (cc/min)	Reference Std. Flow Reading (cc/min)			Avg. (cc/min)	%Error acceptance	Acceptable range (cc/min)	Evaluation (Pass/ Fail)
	1	2	3				
Low Flow							
20	19.9	19.7	19.8	19.8	5%	19 - 21	Passed
50	51.7	50.8	50.2	50.9	5%	48 - 53	Passed
100	99.4	99.7	99.8	99.6	5%	95 - 105	Passed
200	199.2	199.5	200.2	199.6	5%	190 - 210	Passed
High Flow							
500	498.3	498.5	498.2	498.3	3%	485 - 515	Passed
1000	1010.3	1011.1	1009.5	1010.3	3%	970 - 1030	Passed
2000	1994.9	1994.5	1995.1	1994.8	3%	1940 - 2060	Passed
2500	2512.2	2512.8	2513.8	2512.9	3%	2425 - 2575	Passed

----- END OF REPORT -----

Calibrated By: นันทก

(Mr.Natchapon Thamklang)

RYG Field Services Scientist (1)

Issue date : 06-Apr-25

Approved By: Supot S

(Mr.Supot Salamteh)

RYG Field Services Section Head

Certificate of System Qualification

GC-OQ

System ID: GC-6_CN11461066
Organization Name: ALS Laboratory Group (Thailand) Co., Ltd.
Organization Location: 104 Soi 40 Phatthanakan Rd, Khwang Suan Luang, Khet Suan Luang, Bangkok 10250

Date: October 22, 2024 9:27:05 AM
EQP Name: AgilentRecommended
EQP Revision: GC.02.53
Overall Qualification Status: Pass

REVIEW BY Jinda K.
APPROVED BY Tamraton M.
NEXT CAL. DATE 22 Apr 2026

CDS Logon Verification - GC

Logon: Saenguthai Tarak

Overall CDS Logon Verification - GC Test Status

Pass

System Inspection and Basic Safety and Operation

Name: 7890

Setpoint Status: Pass

Overall System Inspection and Basic Safety and Operation Test Status

Pass

Inlet Pressure Decay

Name: 7890

Front SSL

Setpoint Status:

Pass

Pressure: 25.0 psi

Pressure Change: 0.0 psi /5 minutes

Agilent Recommended: ≥ -2.0 and ≤ 0.5

Date: October 22, 2024 9:27:05 AM
System ID: GC-6_CN11461066

Overall Inlet Pressure Decay Test Status

Pass

Inlet Pressure Accuracy

Name:

7890

Front

SSL

Setpoint Status:

Pass

Setpoint

Actual

Inlet Pressure:

25.0

psi

25.07

psi

Accuracy:

0.1

psi

Agilent Recommended:

<=

1.2

Overall Inlet Pressure Accuracy Test Status

Pass

Inlet Pressure Decay

Name:

7890

Back

SSL

Setpoint Status:

Pass

Pressure:

25.0

psi

Pressure Change:

0.0

psi

/5 minutes

Agilent Recommended:

>=

-2.0

and

<=

0.5

Overall Inlet Pressure Decay Test Status

Pass

Inlet Pressure Accuracy

Name:

7890

Back

SSL

Date: October 22, 2024 9:27:05 AM

System ID: GC-6_CN11461066

Setpoint Status:

Pass

	Setpoint		Actual	
Inlet Pressure:	25.0	psi	25.06	psi
Accuracy:			0.1	psi
Agilent Recommended:			<= 1.2	

Overall Inlet Pressure Accuracy Test Status

Pass

Detector Flow Accuracy

Name:

7890

Front

FID

Setpoint Status:

Pass

Flow Type:

Fuel

Setpoint:

30.0

mL/min

Measured Flow:

28.8

mL/min

Accuracy:

1.2

mL/min

Agilent Recommended:

<=

10.0

% setpoint

(

3.0

mL/min

)

Limit is percentage of setpoint or 0.5 mL/minute, whichever is largest.

Setpoint Status:

Pass

Flow Type:

Oxidizer

Setpoint:

400.0

mL/min

Measured Flow:

392

mL/min

Accuracy:

8.0

mL/min

Agilent Recommended:

<=

10.0

% setpoint

(

40.0

mL/min

)

Limit is percentage of setpoint or 0.5 mL/minute, whichever is largest.

Setpoint Status:

Pass

Flow Type:

Makeup

Setpoint:

25.0

mL/min

Measured Flow:

25.4

mL/min

Accuracy:

0.4

mL/min

Agilent Recommended:

<=

10.0

% setpoint

(

2.5

mL/min

)

Limit is percentage of setpoint or 0.5 mL/minute, whichever is largest.

Date:

October 22, 2024 9:27:05 AM

System ID:

GC-6_CN11461066

Overall Detector Flow Accuracy Test Status

Pass

Detector Flow Accuracy

Name:

7890

Back

FID

Setpoint Status:

Pass

Flow Type:

Fuel

Setpoint:

30.0

mL/min

Measured Flow:

30.8

mL/min

Accuracy:

0.8

mL/min

Agilent Recommended:

<=

10.0

% setpoint

(

3.0

mL/min

)

Limit is percentage of setpoint or 0.5 ml/minute, whichever is largest.

Setpoint Status:

Pass

Flow Type:

Oxidizer

Setpoint:

400.0

mL/min

Measured Flow:

393

mL/min

Accuracy:

7.0

mL/min

Agilent Recommended:

<=

10.0

% setpoint

(

40.0

mL/min

)

Limit is percentage of setpoint or 0.5 ml/minute, whichever is largest.

Setpoint Status:

Pass

Flow Type:

Makeup

Setpoint:

25.0

mL/min

Measured Flow:

25.2

mL/min

Accuracy:

0.2

mL/min

Agilent Recommended:

<=

10.0

% setpoint

(

2.5

mL/min

)

Limit is percentage of setpoint or 0.5 ml/minute, whichever is largest.

Overall Detector Flow Accuracy Test Status

Pass

GC Oven Temperature Accuracy

Name:

7890

Date:

October 22, 2024 9:27:05 AM

System ID:

GC-6_CN11461066

Setpoint Status:

Pass

Zone:

Oven

Setpoint/Actual

Temperature:

230.0 230.3 °C

Accuracy:

0.3 °C

Agilent Recommended:

>= -1.0 % setpoint in K (-5.0 °C)

<= 1.0 % setpoint in K (5.0 °C)

Setpoint Status:

Pass

Zone:

Oven

Setpoint/Actual

Temperature:

100.0 100.0 °C

Accuracy:

0.0 °C

Agilent Recommended:

>= -1.0 % setpoint in K (-3.7 °C)

<= 1.0 % setpoint in K (3.7 °C)

Overall GC Oven Temperature Accuracy Test Status

Pass

GC Oven Temperature Stability

Name:

7890

Setpoint Status:

Pass

Setpoint/Average

Temperature:

100.0 100.0167 °C

Stability:

0.1 °C

Agilent Recommended:

<= 0.5

Overall GC Oven Temperature Stability Test Status

Pass

Scouting Run

Tested Combination1

Front

SSL

/ Front

FID

Injection Tower

Name:

7693A

Date:

October 22, 2024 9:27:05 AM

System ID:

GC-6_CN11461066

Setpoint Status:Completed

Injection Volume on Column:1.0uL

Overall Scouting Run Status

Completed

Noise and Drift

Tested Combination1	Front	SSL	/ Front	FID
Name:	7890			
Setpoint Status:	Pass			
Base Signal:	14.05	pA		
	ASTM Noise		Drift	
	pA		pA/Hr	
	0.05		0.03	
Agilent Recommended:	<= 0.10		<= 2.50	
Status:	Pass		Pass	

Overall Noise and Drift Test Status

Pass

Injection Precision

Tested Combination1	Front	SSL	/ Front	FID	
Name:	7693A				
Setpoint Status:	Pass				
Injection Volume on Column:	1.0	uL			
Area RSD:	0.30	%	Retention Time RSD:	0.63	%
Agilent Recommended:	<= 3.00		<= 1.00		

Overall Injection Precision Test Status

Pass

Signal to Noise

Tested Combination1	Front	SSL	/ Front	FID
Injection Tower				
Name:	7890			
Setpoint Status:	Pass			
Signal to Noise:	11078525			
Agilent Recommended:	>= 300000			
Overall Signal to Noise Test Status				
Pass				

Scouting Run

Tested Combination2	Back	SSL	/ Back	FID
Injection Tower				
Name:	7693A			
Setpoint Status:	Completed			
Injection Volume on Column:	1.0 uL			
Overall Scouting Run Status				
Completed				

Noise and Drift

Tested Combination2	Back	SSL	/ Back	FID
Name:	7890			
Setpoint Status:	Pass			
Base Signal:	13.79 pA			
ASTM Noise				
pA				
0.05				
<= 0.10				
Pass				
Drift				
pA/Hr				
0.01				
<= 2.50				
Pass				
Agilent Recommended:	<= 0.10			
Status:	Pass			

Overall Noise and Drift Test Status

Pass

Injection Precision

Tested Combination2

Back

SSL

/ Back

FID

Name:

7693A

Setpoint Status:

Pass

Injection Volume on Column:

1.0 uL

Area RSD:

1.06 %

Retention Time RSD:

0.93 %

Agilent Recommended:

<= 3.00

<= 1.00

Overall Injection Precision Test Status

Pass

Signal to Noise

Tested Combination2

Back

SSL

/ Back

FID

Injection Tower

Name:

7890

Setpoint Status:

Pass

Signal to Noise:

1771221

Agilent Recommended:

>= 300000

Overall Signal to Noise Test Status

Pass

Instrument Details

Purpose

This section describes the as found system configuration.

Details

System

System ID	GC-6_CN11461066
Manufacturer	Agilent Technologies
Name	7890
Flow Data Input	Manual Data
Temperature Data Input	Manual Data or Other Data Logging

Tested Combination1

Injection Technique	Injection Tower
Sampler Identifier	Sampler 1
Inlet	Front
Detector	Front
LTM Included?	No

Tested Combination2

Injection Technique	Injection Tower
Sampler Identifier	Sampler 2
Inlet	Back
Detector	Back
LTM Included?	No

Sampler 1

Manufacturer	Agilent Technologies
Type	Injection Tower
Name	7693A
Model Number	G4513A
Serial Number	CNCN10340103
Firmware Revision	A.11.06
Usage	Sample Injection
Location	Front
Syringe Volume (µL)	10

Sampler 2

Manufacturer	Agilent Technologies
Type	Injection Tower
Name	7693A
Model Number	G4513A
Serial Number	CN16280128
Firmware Revision	A.11.06
Usage	Sample Injection
Location	Back
Syringe Volume (µL)	10

Sampler 3

Manufacturer	Agilent Technologies
Type	Tray
Name	7693A
Model Number	G4514A
Serial Number	CN15380030
Firmware Revision	A.11.03
Vial Heater	Not installed

Mainframe 1

Manufacturer	Agilent Technologies
Name	7890
Model Number	G3440A
Serial Number	CN11461066
Firmware Revision	A.01.16
Oven Type	Standard

Inlet 1

Manufacturer	Agilent Technologies
Name	7890
Type	SSL
Location	Front
Carrier Gas	Helium
Control Type	Electronic Pressure Control (EPC)
Purged Inlet	Yes

Inlet 2

Manufacturer	Agilent Technologies
Name	7890
Type	SSL
Location	Back
Carrier Gas	Helium
Control Type	Electronic Pressure Control (EPC)
Purged Inlet	Yes

Detector 1

Manufacturer	Agilent Technologies
Name	7890
Type	FID
Adapter	Capillary
Control Type	Electronic Pressure Control (EPC)
Location	Front
Makeup Gas	Nitrogen

Detector 2

Manufacturer	Agilent Technologies
Name	7890
Type	FID
Adapter	Capillary
Control Type	Electronic Pressure Control (EPC)
Location	Back
Makeup Gas	Nitrogen

Electronic Signature

Purpose

This signature page was created and published because the ACE sign-off action was executed, which is valid for the entire document, including attachments. The ACE sign-off is an electronic signature that requires two distinct identification components: unique username and personal password. The Agilent representative who has delivered this service understands the meaning and legal status of an electronic signature. As a trained official operator, the Agilent representative has a unique password and logon to access ACE and electronically sign this document. (Other e-signatures can be applied to this document using a Document Content Management or other suitable method defined in your data access and control procedures.)

Details

Full Name of Signer:	Saenguthai Tarak
Logged On User Name:	saenguthai.tarak@non.agilent.com
Signature Creation Date:	October 22, 2024
Reason for Signature:	Executed protocol and published this original version of document

Regulatory Disclaimer

This document provides a protocol to verify and record instrument configuration and evidence of proper operation. It has been prepared from our interpretation of applicable regulations as well as industry best practices. The document is designed to provide an important component of a complete compliance package. Validation depends upon many factors and use of this protocol alone does not assure compliance. Agilent Technologies makes no promises or representations as to its sufficiency for any specific regulatory program.

Warranty

Agilent Technologies makes no warranty of any kind to this material, including but not limited to, the implied warranties or merchantability and fitness for a particular purpose. Agilent Technologies shall not be liable for errors contained herein or for incidental or consequential damages in connection with the furnishing, performance, or use of this material.

User Name: saenguthai.tarak

System Id: GC-6_CN11461066

Report Generated by Hostname: LAPTOP-CQ3SKOMV

Print Date: October 22, 2024 9:27:06 AM

2024_ALS_GC-6_CN11461066_OQHW Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
October 21, 2024 3:16:06 PM	Audit	SessionCreated	Session	None
October 21, 2024 3:16:07 PM	Start	Configuration	Session	None
October 21, 2024 3:16:07 PM	Audit	Entitlement	Licensing	User is Nonpaying and does not require an unlock code
October 21, 2024 3:22:40 PM	Audit	EqpLoaded	Session	EQP details for primary technique [Gc] - File path: [ProtocolPacks/Gc/Configurations/02.53/Gc.02.53.eqp], EQP File Name: [Gc.02.53.eqp], EQP Name: [AgilentRecommended], Protocol Revision :[Gc.02.53]
October 21, 2024 3:22:44 PM	End	Configuration	Session	None
October 21, 2024 3:22:47 PM	Start	Qualification	Session	OQ
October 21, 2024 3:22:48 PM	Start	Execution	CDS Logon Verification - GC - 7890: - Qualitative test	None
October 21, 2024 3:23:35 PM	End	Execution	CDS Logon Verification - GC - 7890: - Qualitative test	Run Count : 1
October 21, 2024 3:23:45 PM	Start	Execution	System Inspection and Basic Safety and Operation - 7890: - Qualitative Test - No setpoints associated	None
October 21, 2024 3:23:59 PM	End	Execution	System Inspection and Basic Safety and Operation - 7890: - Qualitative Test - No setpoints associated	Run Count : 1

User Name: saenguthai.tarak
Report Generated by Hostname: LAPTOP-CQ3SKOMV

System Id: GC-6_CN11461066
Print Date: October 22, 2024 9:27:06 AM

2024_ALS_GC-6_CN11461066_OQHW Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
October 21, 2024 3:24:01 PM	Start	Execution	Inlet Pressure Decay - Front SSL: - Pressure Controlled Inlet - S: 25.0 psi - L: >= -2.0 psi and <= 0.5 psi	None
October 21, 2024 3:25:26 PM	End	Execution	Inlet Pressure Decay - Front SSL: - Pressure Controlled Inlet - S: 25.0 psi - L: >= -2.0 psi and <= 0.5 psi	Run Count : 1
October 21, 2024 3:25:28 PM	Start	Execution	Inlet Pressure Accuracy - Front SSL: - Pressure Controlled Inlet - S: 25.0 psi - L: <= 1.2 psi	None
October 21, 2024 3:25:32 PM	End	Execution	Inlet Pressure Accuracy - Front SSL: - Pressure Controlled Inlet - S: 25.0 psi - L: <= 1.2 psi	Run Count : 1
October 21, 2024 3:25:50 PM	Start	Execution	Inlet Pressure Decay - Back SSL: - Pressure Controlled Inlet - S: 25.0 psi - L: >= -2.0 psi and <= 0.5 psi	None
October 21, 2024 3:26:01 PM	End	Execution	Inlet Pressure Decay - Back SSL: - Pressure Controlled Inlet - S: 25.0 psi - L: >= -2.0 psi and <= 0.5 psi	Run Count : 1
October 21, 2024 3:26:05 PM	Start	Execution	Inlet Pressure Accuracy - Back SSL: - Pressure Controlled Inlet - S: 25.0 psi - L: <= 1.2 psi	None
October 21, 2024 3:26:10 PM	End	Execution	Inlet Pressure Accuracy - Back SSL: - Pressure Controlled Inlet - S: 25.0 psi - L: <= 1.2 psi	Run Count : 1
October 21, 2024 3:26:12 PM	Start	Execution	Detector Flow Accuracy - Front FID: - Type : Fuel - S: 30.0 mL/min - L: <= 10.0% setpoint	None

User Name: saenguthai.tarak

System Id: GC-6_CN11461066

Report Generated by Hostname: LAPTOP-CQ3SKOMV

Print Date: October 22, 2024 9:27:06 AM

2024_ALS_GC-6_CN11461066_OQHW Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
October 21, 2024 3:26:50 PM	Audit	Data	Detector Flow Accuracy - Front FID: - Type : Fuel - S: 30.0 mL/min - L: <= 10.0% setpoint	Manual Data Entry
October 21, 2024 3:26:53 PM	End	Execution	Detector Flow Accuracy - Front FID: - Type : Fuel - S: 30.0 mL/min - L: <= 10.0% setpoint	Run Count : 1
October 21, 2024 3:26:54 PM	Start	Execution	Detector Flow Accuracy - Front FID: - Type : Oxidizer - S: 400.0 mL/min - L: <= 10.0% setpoint	None
October 21, 2024 3:27:10 PM	Audit	Data	Detector Flow Accuracy - Front FID: - Type : Oxidizer - S: 400.0 mL/min - L: <= 10.0% setpoint	Manual Data Entry
October 21, 2024 3:27:13 PM	End	Execution	Detector Flow Accuracy - Front FID: - Type : Oxidizer - S: 400.0 mL/min - L: <= 10.0% setpoint	Run Count : 1
October 21, 2024 3:29:11 PM	Start	Execution	Detector Flow Accuracy - Front FID: - Type : Makeup - S: 25.0 mL/min - L: <= 10.0% setpoint	None
October 21, 2024 3:29:27 PM	Audit	Data	Detector Flow Accuracy - Front FID: - Type : Makeup - S: 25.0 mL/min - L: <= 10.0% setpoint	Manual Data Entry
October 21, 2024 3:29:29 PM	End	Execution	Detector Flow Accuracy - Front FID: - Type : Makeup - S: 25.0 mL/min - L: <= 10.0% setpoint	Run Count : 1
October 21, 2024 3:29:30 PM	Start	Execution	Detector Flow Accuracy - Back FID: - Type : Fuel - S: 30.0 mL/min - L: <= 10.0% setpoint	None
October 21, 2024 3:29:47 PM	Audit	Data	Detector Flow Accuracy - Back FID: - Type : Fuel - S: 30.0 mL/min - L: <= 10.0% setpoint	Manual Data Entry
October 21, 2024 3:29:52 PM	End	Execution	Detector Flow Accuracy - Back FID: - Type : Fuel - S: 30.0 mL/min - L: <= 10.0% setpoint	Run Count : 1

Page 3 / 10

User Name: saenguthai.tarak
Report Generated by Hostname: LAPTOP-CQ3SKOMV

System Id: GC-6_CN11461066
Print Date: October 22, 2024 9:27:06 AM

2024_ALS_GC-6_CN11461066_OQHW Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
October 21, 2024 3:29:54 PM	Start	Execution	Detector Flow Accuracy - Back FID: - Type : Oxidizer - S: 400.0 mL/min - L: <= 10.0% setpoint	None
October 21, 2024 3:30:07 PM	Audit	Data	Detector Flow Accuracy - Back FID: - Type : Oxidizer - S: 400.0 mL/min - L: <= 10.0% setpoint	Manual Data Entry
October 21, 2024 3:30:09 PM	End	Execution	Detector Flow Accuracy - Back FID: - Type : Oxidizer - S: 400.0 mL/min - L: <= 10.0% setpoint	Run Count : 1
October 21, 2024 3:30:11 PM	Start	Execution	Detector Flow Accuracy - Back FID: - Type : Makeup - S: 25.0 mL/min - L: <= 10.0% setpoint	None
October 21, 2024 3:30:34 PM	Audit	Data	Detector Flow Accuracy - Back FID: - Type : Makeup - S: 25.0 mL/min - L: <= 10.0% setpoint	Manual Data Entry
October 21, 2024 3:30:37 PM	End	Execution	Detector Flow Accuracy - Back FID: - Type : Makeup - S: 25.0 mL/min - L: <= 10.0% setpoint	Run Count : 1
October 21, 2024 3:30:38 PM	Start	Execution	GC Oven Temperature Accuracy - 7890: - Temperature : Oven - S: 230.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	None
October 21, 2024 3:31:55 PM	Audit	Data	GC Oven Temperature Accuracy - 7890: - Temperature : Oven - S: 230.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	Manual Data Entry
October 21, 2024 3:31:57 PM	End	Execution	GC Oven Temperature Accuracy - 7890: - Temperature : Oven - S: 230.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	Run Count : 1

User Name: saenguthai.tarak

System Id: GC-6_CN11461066

Report Generated by Hostname: LAPTOP-CQ3SKOMV

Print Date: October 22, 2024 9:27:06 AM

2024_ALS_GC-6_CN11461066_OQHW Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
October 21, 2024 3:31:59 PM	Start	Execution	GC Oven Temperature Accuracy - 7890: - Temperature : Oven - S: 100.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	None
October 21, 2024 3:34:37 PM	Audit	Data	GC Oven Temperature Accuracy - 7890: - Temperature : Oven - S: 100.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	Manual Data Entry
October 21, 2024 3:34:39 PM	End	Execution	GC Oven Temperature Accuracy - 7890: - Temperature : Oven - S: 100.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	Run Count : 1
October 21, 2024 3:34:42 PM	Start	Execution	GC Oven Temperature Stability - 7890: - Temperature : Oven - S: 100.0°C - L: <= 0.5°C	None
October 21, 2024 3:39:05 PM	Audit	Data	GC Oven Temperature Stability - 7890: - Temperature : Oven - S: 100.0°C - L: <= 0.5°C	Manual Data Entry
October 21, 2024 3:39:07 PM	End	Execution	GC Oven Temperature Stability - 7890: - Temperature : Oven - S: 100.0°C - L: <= 0.5°C	Run Count : 1
October 21, 2024 3:39:33 PM	Start	Execution	GC Scouting Run - Injection Tower, Front SSL, Front FID: - Part of System Preparation - No limits associated	None
October 21, 2024 3:40:12 PM	Audit	AceClosed	Session	None
October 22, 2024 8:55:47 AM	Audit	AceRestarted	Session	None
October 22, 2024 8:55:50 AM	Audit	SessionReloaded	Session	None
October 22, 2024 8:56:02 AM	Start	Qualification	Session	OQ

Page 5 / 10

User Name: saenguthai.tarak
Report Generated by Hostname: LAPTOP-CQ3SKOMV

System Id: GC-6_CN11461066
Print Date: October 22, 2024 9:27:06 AM

2024_ALS_GC-6_CN11461066_OQHW Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
October 22, 2024 8:56:02 AM	Start	Execution	GC Scouting Run - Injection Tower, Front SSL, Front FID: - Part of System Preparation - No limits associated	None
October 22, 2024 8:56:46 AM	Audit	Data	GC Scouting Run - Injection Tower, Front SSL, Front FID: - Part of System Preparation - No limits associated	Data files Path : G:\Data\Front\Front_SC10.D\FID1A.ch
October 22, 2024 8:57:25 AM	End	Execution	GC Scouting Run - Injection Tower, Front SSL, Front FID: - Part of System Preparation - No limits associated	Run Count : 1
October 22, 2024 8:57:39 AM	Start	Execution	Noise and Drift - Front FID: - Detector FID - L (Noise): <= 0.10 pA - L (Drift): <= 2.50 pA/hour	None
October 22, 2024 8:58:03 AM	Audit	Data	Noise and Drift - Front FID: - Detector FID - L (Noise): <= 0.10 pA - L (Drift): <= 2.50 pA/hour	Data files Path : G:\Data\Front\Front_ND10.D\FID1A.ch
October 22, 2024 8:58:37 AM	End	Execution	Noise and Drift - Front FID: - Detector FID - L (Noise): <= 0.10 pA - L (Drift): <= 2.50 pA/hour	Run Count : 1
October 22, 2024 8:58:40 AM	Start	Execution	Injection Precision - Injection Tower, Front SSL, Front FID: - GC - L (Area): <= 3.00% - L (Ret. Time): <= 1.00%	None
October 22, 2024 8:59:06 AM	Audit	Data	DataManager	DataManager was in a data verification state but the user chose to start over

User Name: saenguthai.tarak

System Id: GC-6_CN11461066

Report Generated by Hostname: LAPTOP-CQ3SKOMV

Print Date: October 22, 2024 9:27:06 AM

2024_ALS_GC-6_CN11461066_OQHW Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
October 22, 2024 9:01:43 AM	Audit	Data	Injection Precision - Injection Tower, Front SSL, Front FID: - GC - L (Area): <= 3.00% - L (Ret. Time): <= 1.00%	Data files Path : G:\Data\Front\Front_IP0105.D\FID1A.ch
October 22, 2024 9:01:43 AM	Audit	Data	Injection Precision - Injection Tower, Front SSL, Front FID: - GC - L (Area): <= 3.00% - L (Ret. Time): <= 1.00%	Data files Path : G:\Data\Front\Front_IP0106.D\FID1A.ch
October 22, 2024 9:01:43 AM	Audit	Data	Injection Precision - Injection Tower, Front SSL, Front FID: - GC - L (Area): <= 3.00% - L (Ret. Time): <= 1.00%	Data files Path : G:\Data\Front\Front_IP0107.D\FID1A.ch
October 22, 2024 9:01:43 AM	Audit	Data	Injection Precision - Injection Tower, Front SSL, Front FID: - GC - L (Area): <= 3.00% - L (Ret. Time): <= 1.00%	Data files Path : G:\Data\Front\Front_IP0108.D\FID1A.ch
October 22, 2024 9:01:43 AM	Audit	Data	Injection Precision - Injection Tower, Front SSL, Front FID: - GC - L (Area): <= 3.00% - L (Ret. Time): <= 1.00%	Data files Path : G:\Data\Front\Front_IP0109.D\FID1A.ch
October 22, 2024 9:01:43 AM	Audit	Data	Injection Precision - Injection Tower, Front SSL, Front FID: - GC - L (Area): <= 3.00% - L (Ret. Time): <= 1.00%	Data files Path : G:\Data\Front\Front_IP0110.D\FID1A.ch
October 22, 2024 9:02:11 AM	End	Execution	Injection Precision - Injection Tower, Front SSL, Front FID: - GC - L (Area): <= 3.00% - L (Ret. Time): <= 1.00%	Run Count : 1
October 22, 2024 9:02:16 AM	Start	Execution	Signal to Noise - Injection Tower, Front SSL, Front FID: - Detector FID - L: >= 300000	None
October 22, 2024 9:02:34 AM	Audit	Data	Signal to Noise - Injection Tower, Front SSL, Front FID: - Detector FID - L: >= 300000	Data files Path : G:\Data\Front\Front_SN01.D\FID1A.ch

Page 7 / 10

User Name: saenguthai.tarak

System Id: GC-6_CN11461066

Report Generated by Hostname: LAPTOP-CQ3SKOMV

Print Date: October 22, 2024 9:27:06 AM

2024_ALS_GC-6_CN11461066_OQHW Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
October 22, 2024 9:02:54 AM	End	Execution	Signal to Noise - Injection Tower, Front SSL, Front FID: - Detector FID - L: ≥ 300000	Run Count : 1
October 22, 2024 9:03:00 AM	Start	Execution	GC Scouting Run - Injection Tower, Back SSL, Back FID: - Part of System Preparation - No limits associated	None
October 22, 2024 9:03:31 AM	Audit	Data	GC Scouting Run - Injection Tower, Back SSL, Back FID: - Part of System Preparation - No limits associated	Data files Path : G:\Data\Back\Back_SC01.D\FID2B.ch
October 22, 2024 9:04:03 AM	End	Execution	GC Scouting Run - Injection Tower, Back SSL, Back FID: - Part of System Preparation - No limits associated	Run Count : 1
October 22, 2024 9:04:06 AM	Start	Execution	Noise and Drift - Back FID: - Detector FID - L (Noise): ≤ 0.10 pA - L (Drift): ≤ 2.50 pA/hour	None
October 22, 2024 9:08:56 AM	Audit	Data	Noise and Drift - Back FID: - Detector FID - L (Noise): ≤ 0.10 pA - L (Drift): ≤ 2.50 pA/hour	Data files Path : G:\Data\Back\Back_ND013.D\FID2B.ch
October 22, 2024 9:09:13 AM	End	Execution	Noise and Drift - Back FID: - Detector FID - L (Noise): ≤ 0.10 pA - L (Drift): ≤ 2.50 pA/hour	Run Count : 1
October 22, 2024 9:09:26 AM	Start	Execution	Injection Precision - Injection Tower, Back SSL, Back FID: - GC - L (Area): $\leq 3.00\%$ - L (Ret. Time): $\leq 1.00\%$	None

User Name: saenguthai.tarak

System Id: GC-6_CN11461066

Report Generated by Hostname: LAPTOP-CQ3SKOMV

Print Date: October 22, 2024 9:27:06 AM

2024_ALS_GC-6_CN11461066_OQHW Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
October 22, 2024 9:10:44 AM	Audit	Data	Injection Precision - Injection Tower, Back SSL, Back FID: - GC - L (Area): <= 3.00% - L (Ret. Time): <= 1.00%	Data files Path : G:\Data\Back\Back_IP0111.D \FID2B.ch
October 22, 2024 9:10:44 AM	Audit	Data	Injection Precision - Injection Tower, Back SSL, Back FID: - GC - L (Area): <= 3.00% - L (Ret. Time): <= 1.00%	Data files Path : G:\Data\Back\Back_IP0112.D \FID2B.ch
October 22, 2024 9:10:44 AM	Audit	Data	Injection Precision - Injection Tower, Back SSL, Back FID: - GC - L (Area): <= 3.00% - L (Ret. Time): <= 1.00%	Data files Path : G:\Data\Back\Back_IP0113.D \FID2B.ch
October 22, 2024 9:10:44 AM	Audit	Data	Injection Precision - Injection Tower, Back SSL, Back FID: - GC - L (Area): <= 3.00% - L (Ret. Time): <= 1.00%	Data files Path : G:\Data\Back\Back_IP0114.D \FID2B.ch
October 22, 2024 9:10:44 AM	Audit	Data	Injection Precision - Injection Tower, Back SSL, Back FID: - GC - L (Area): <= 3.00% - L (Ret. Time): <= 1.00%	Data files Path : G:\Data\Back\Back_IP0115.D \FID2B.ch
October 22, 2024 9:10:44 AM	Audit	Data	Injection Precision - Injection Tower, Back SSL, Back FID: - GC - L (Area): <= 3.00% - L (Ret. Time): <= 1.00%	Data files Path : G:\Data\Back\Back_IP0116.D \FID2B.ch
October 22, 2024 9:11:15 AM	End	Execution	Injection Precision - Injection Tower, Back SSL, Back FID: - GC - L (Area): <= 3.00% - L (Ret. Time): <= 1.00%	Run Count : 1
October 22, 2024 9:11:23 AM	Start	Execution	Signal to Noise - Injection Tower, Back SSL, Back FID: - Detector FID - L: >= 300000	None
October 22, 2024 9:11:45 AM	Audit	Data	Signal to Noise - Injection Tower, Back SSL, Back FID: - Detector FID - L: >= 300000	Data files Path : G:\Data\Back\Back_SN01.D \FID2B.ch

Page 9 / 10

User Name: saenguthai.tarak

System Id: GC-6_CN11461066

Report Generated by Hostname: LAPTOP-CQ3SKOMV

Print Date: October 22, 2024 9:27:06 AM

2024_ALS_GC-6_CN11461066_OQHW Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
October 22, 2024 9:12:08 AM	End	Execution	Signal to Noise - Injection Tower, Back SSL, Back FID: - Detector FID - L: >= 300000	Run Count : 1
October 22, 2024 9:12:15 AM	End	Qualification	Session	OQ
October 22, 2024 9:12:15 AM	Start	Reporting	Session	None
October 22, 2024 9:24:09 AM	Audit	Reporting	Session	Report Generated : Certificate
October 22, 2024 9:25:56 AM	Audit	Reporting	Session	Report Generated : Report

Certificate of Calibration

Customer

Name : ALS Laboratory Group Thailand Co., Ltd. **Certificate No** : 25-ACT-042
Address : 104 Soi Phatthanakan 40, Phatthanakan Road, Suan Luang, **Request No** : Req-2025-0604
Bangkok 10250

Unit Under Calibration Details

Measurement item : Acoustic Calibrator Class : 1
Manufacturer : RION Range : 94 dB / 1000 Hz
Model : NC-75 Instrument Status : Used
Serial Number : 35002736
ID : RYG_FS0496

Calibration Environment and Details

Temperature : (23 \pm 2 $^{\circ}$ C)
Humidity : (50 \pm 20 %RH)
Barometric Pressure : (1013 \pm 10.0 hPa)
Received Date : 6 March 2025
Calibration Date : 19 March 2025
Location of Calibration : LAB 1 Acoustic
Calibration Procedure : In-house method CP-ACT-02 based on IEC 60942:2017 Electroacoustics - Sound calibrators

REVIEW BY 

APPROVED BY 


NEXT CAL DATE 19/03/26


Reference Standard	Model	Serial Number	Traceable	Due Calibration
Sound Calibrator	SV 35A	58079	EEI	12 June 2025
THD Multimeter	2015	1047765	NIMT	4 February 2026

Traceability : This certificate provides traceability of measurement to recognized national standard, and to the realization of the international System of Units (SI).

Note

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor $k=2$, providing a level of confidence approximately 95 %.

Calibrated By : 
Mr. Noppadon Luangart
Service Calibration Engineer

Approved By : 
Mr. Pacit Mathavorn
Calibration Engineer Supervisor

Issue Date : 19 March 2025

Certificate No : 25-ACT-042

Request No : Req-2025-0604

Sound pressure level

Calibration Results : Without Adjustment

Calibration Range (dB)	Without Adjustment (dB)		Adjustment (dB)		Uncertainty (± dB)	Acceptance limit Class 1 (± dB)	Result
	Measured	Deviated value	Measured	Deviated value			
94 dB / 1000 Hz	94.06	0.06	-	-	0.13	0.25	Pass

Frequency of Sound pressure level

Calibration Range (Hz)	Without Adjustment		Adjustment		Uncertainty (± %)	Acceptance limit Class 1 (± %)	Result
	Measured (Hz)	Deviated	Measured (Hz)	Deviated			
94 dB / 1000 Hz	1000.00	0.00	-	-	0.01	0.70	Pass

Total Harmonic Distortion plus Noise of Sound pressure level (THD+N %)

Calibration Range (Hz)	Without Adjustment	Adjustment	Uncertainty (± %)	Acceptance limit Class 1 (± %)	Result
	Measured (%)	Measured (%)			
94 dB / 1000 Hz	0.98	-	0.40	2.5	Pass

Note :

Function	Maximum-permitted Uncertainty of measurement
Sound pressure level	0.15 dB
Frequency	0.20%
Total distortion+noise	0.50%

- Acceptance limit was IEC60942:2017 Class 1

- The calibration results exclude the calibrator pressure correction

- The calibration results exclude the microphone volume correction

Certificate No : 25-ACT-042

Request No : Req-2025-0604

Decision Rule for Statements of Conformity


The standard decision rule employed for the statements of conformity to each calibration result will be applied using ILAC-G8:09/2019; Guidelines on the Reporting of Compliance with Specification as following Fig. and statements

Pass = The measurement result plus the expanded uncertainty with a 95% coverage probability were within the limit.

Pass¹ = The measurement result was within the limit. However, a portion of the expanded uncertainty of measurement at 95% exceeds the limit.

Fail¹ = The measurement result was out of the limit. However, a portion of the expanded uncertainty of measurement at 95% is within the limit.

Fail = The measurement result plus the expanded uncertainty with a 95% coverage probability were outside the limit.

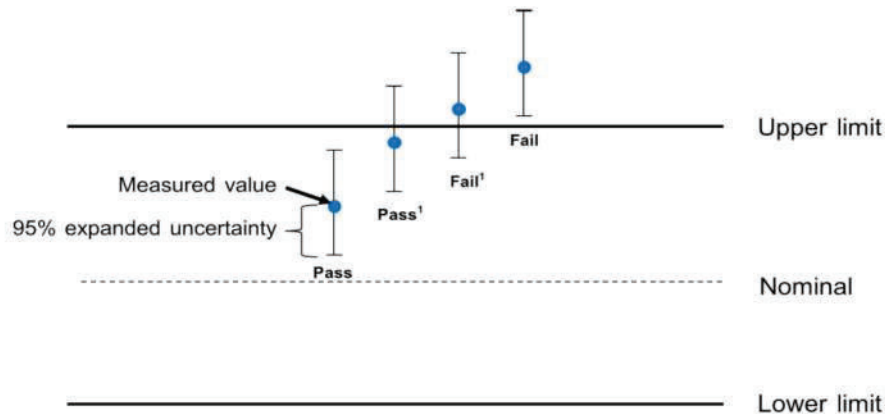

End of Calibration

Cert. No. : ACL25107

Pages : 1 of 8

Calibration Certificate

Equipment : SOUND LEVEL METER
Manufacturer : RION
Model : NL-42 / Microphone UC-52 / Preamplifier NH-24
Serial No.: 00900071 / 188464 / 01733
ID No.: RYG_FS0492

Condition As Found : GOOD

Customer : ALS LABORATORY GROUP (THAILAND) CO., LTD.
104 PHATTHANAKAN 40, PHATTHANAKAN ROAD,
KHWANG PHATTHANAKAN, KHET SUAN LUANG,
BANGKOK, 10250 THAILAND.

Location : -
Ambient Temperature : (23.0 \pm 3) °C
Pressure : (101.3 \pm 3) kPa
Relative Humidity : (50.0 \pm 20) %

Received Date : 14 JANUARY 2025
Calibration Date : 27-29 JANUARY 2025
Date of Issue : 30 JANUARY 2025

REVIEW BY *Supt S*

APPROVED BY *[Signature]*

NEXT CAL DATE..... 26/ 01/ 2026

Calibrated by :

Nathakorn Pisutpaisan

Approved by :

[Signature]
(Thanakul Petchurai)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

Cert. No. : ACL25107
Job No. : VC68AC0064
Pages : 2 of 8

Calibration Procedure : CP-AC-01

Calibration Method :

This equipment was calibrated by follow on IEC-61672-3 (2013) Standard for sound level meter (SLM).

The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.

For tests results of each items were made by observation of each Instruments display and also with SLM's display.

Condition of this result of calibration :

1. Reference Standard Instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
Waveform Generator	33210A	MY48017076	EF-0009-24	05-FEB-25
Waveform Generator	33511B	MY52302742	EF-0007-24	05-FEB-25
Digital Multimeter	33461A	MY53220104	EEL.BP 21/0267	13-FEB-25
Digital Multimeter	33461A	MY53220076	EEL.BP 20/0267	15-FEB-25
Digital Multimeter	34461A	MY60024273	EEL.BP 22/0267	15-FEB-25
Programmable Attenuator	MAT-1070	62100114	EF-0008-24	05-FEB-25
Condenser Microphone	4180	2977900	AA-1001-24	12-FEB-25
Measuring Amplifier	NA-42KAI	34560495	AA-3001-24	05-FEB-25

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is traceable to the international system of unit maintained at :

3.1 National Institute of Metrology (Thailand).

3.2 Thailand Institute of Scientific and Technological Research (TISTR).

T. Ketch.

Cert. No. : ACL25107
Job No. : VC68AC0064
Pages : 3 of 8

Summary of Measurement Result :

Parameter	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	0.2	N/A
2. Self-generated noise	0.2	N/A
3. Acoustical signal tests of frequency weightings		
125 Hz	0.3	0.6
1000 Hz	0.3	0.6
8000 Hz	0.3	0.7
4. Electrical signal tests of frequency weightings		
For 10 Hz to 4 kHz	0.3	0.6
For > 4 kHz to 10 kHz	0.3	0.7
For > 10 kHz to 20 kHz	0.3	1.0
5. Frequency and time weightings at 1 kHz	0.2	0.2
6. Long - term stability	0.1	0.1
7. Level linearity on the reference level range	0.2	0.3
8. Level linearity including the level range control	0.2	0.3
9. Tone burst response	0.2	0.3
10. Peak C sound level	0.2	0.35
11. Overload indication	0.2	0.25
12. High level stability	0.1	0.1

T. Petch.

Cert. No. : ACL25107
Job No. : VC68AC0064
Page : 4 of 8

Result of calibration :

1. Absolute sensitivity

Reference Acoustic Signal (dB)	Measured Value (dB)	Deviation (dB)	Acceptance Limit (dB)
93.9 (93.94)	93.9	0.0	±0.3

2. Self-generated noise

2.1 Normal test

Measured Value (dB)
15.1

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Weighting (dB)
A - weight	12.0
C - weight	18.4
Flat	24.1

3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
125	0.2	0.2	0.2	± 1.5
1000	0.1	0.1	0.1	± 1.0
8000	0.9	0.9	0.9	±5.0

G. Rehn

Cert. No. : ACL25107
Job No. : VC68AC0064
Pages : 5 of 8

4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	0.0	0.0	0.0	±2.0
125	0.0	0.1	0.0	±1.5
250	0.0	0.0	0.0	±1.5
500	0.0	0.0	0.0	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.0	0.0	±2.0
4000	0.0	0.0	0.0	±3.0
8000	0.0	0.1	0.1	±5.0

5. Frequency and time weightings at 1 kHz

5.1 Frequency weightings at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.2
C - weight	94.0	94.0	0.0	± 0.2
Flat	94.0	94.0	0.0	± 0.2

5.2 Time weighting at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	94.0	94.0	0.0	± 0.1
Slow	94.0	94.0	0.0	± 0.1
Leq	94.0	94.0	0.0	± 0.1

6. Long - term stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.3

T. K. K.

Cert. No. : ACL25107

Job No. : VC68AC0064

Pages : 6 of 8

7. Level linearity on the reference level range

Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
137.0	137.0	0.0	± 1.1
136.0	136.0	0.0	± 1.1
135.0	135.0	0.0	± 1.1
134.0	134.0	0.0	± 1.1
133.0	133.0	0.0	± 1.1
132.0	132.0	0.0	± 1.1
131.0	131.0	0.0	± 1.1
129.0	129.0	0.0	± 1.1
124.0	124.0	0.0	± 1.1
119.0	119.0	0.0	± 1.1
114.0	114.0	0.0	± 1.1
109.0	109.0	0.0	± 1.1
104.0	104.0	0.0	± 1.1
99.0	99.0	0.0	± 1.1
94.0	94.0	0.0	± 1.1
89.0	89.0	0.0	± 1.1
84.0	84.0	0.0	± 1.1
79.0	78.9	-0.1	± 1.1
74.0	74.0	0.0	± 1.1
69.0	69.0	0.0	± 1.1
64.0	63.9	-0.1	± 1.1
59.0	59.0	0.0	± 1.1
54.0	53.9	-0.1	± 1.1
49.0	48.9	-0.1	± 1.1
44.0	43.9	-0.1	± 1.1
39.0	38.9	-0.1	± 1.1
34.0	33.9	-0.1	± 1.1
30.0	30.0	0.0	± 1.1
29.0	29.0	0.0	± 1.1
28.0	28.0	0.0	± 1.1
27.0	27.1	0.1	± 1.1
26.0	26.1	0.1	± 1.1
25.0	25.2	0.2	± 1.1

T. Petch.

Cert. No. : ACL25101

Pages : 1 of 8

Calibration Certificate

Equipment : SOUND LEVEL METER
Manufacturer : RION
Model : NL-42 / Microphone UC-52 / Preamplifier NH-24
Serial No.: 01173610 / 143485 / 22619
ID No.: RYG_FS0389

Condition As Found : GOOD

Customer : ALS LABORATORY GROUP (THAILAND) CO., LTD.
104 PHATTHANAKAN 40, PHATTHANAKAN ROAD,
KHWAEANG PHATTHANAKAN, KHET SUAN LUANG,
BANGKOK, 10250 THAILAND.

Location : -
Ambient Temperature : (23.0 \pm 3) °C
Pressure : (101.3 \pm 3) kPa
Relative Humidity : (50.0 \pm 20) %

Received Date : 14 JANUARY 2025
Calibration Date : 27-29 JANUARY 2025
Date of Issue : 30 JANUARY 2025

REVIEW BY *Supt S*

APPROVED BY *[Signature]*

NEXT CAL DATE..... 26/ 01/ 2026

Calibrated by :

Nathakorn Pisutpaisan

Approved by :

[Signature]
(Thanakul Petchurai)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

Cert. No. : ACL25101
Job No. : VC68AC0064
Pages : 2 of 8

Calibration Procedure : CP-AC-01

Calibration Method :

This equipment was calibrated by follow on IEC-61672-3 (2013) Standard for sound level meter (SLM).

The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.

For tests results of each items were made by observation of each Instruments display and also with SLM's display.

Condition of this result of calibration :

1. Reference Standard Instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
Waveform Generator	33210A	MY48017076	EF-0009-24	05-FEB-25
Waveform Generator	33511B	MY52302742	EF-0007-24	05-FEB-25
Digital Multimeter	33461A	MY53220104	EEL.BP 21/0267	13-FEB-25
Digital Multimeter	33461A	MY53220076	EEL.BP 20/0267	15-FEB-25
Digital Multimeter	34461A	MY60024273	EEL.BP 22/0267	15-FEB-25
Programmable Attenuator	MAT-1070	62100114	EF-0008-24	05-FEB-25
Condenser Microphone	4180	2977900	AA-1001-24	12-FEB-25
Measuring Amplifier	NA-42KAI	34560495	AA-3001-24	05-FEB-25

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is traceable to the international system of unit maintained at :

3.1 National Institute of Metrology (Thailand).

3.2 Thailand Institute of Scientific and Technological Research (TISTR).

T. Petch.

Cert. No. : ACL25101
Job No. : VC68AC0064
Pages : 3 of 8

Summary of Measurement Result :

Parameter	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	0.2	N/A
2. Self-generated noise	0.2	N/A
3. Acoustical signal tests of frequency weightings		
125 Hz	0.3	0.6
1000 Hz	0.3	0.6
8000 Hz	0.3	0.7
4. Electrical signal tests of frequency weightings		
For 10 Hz to 4 kHz	0.3	0.6
For > 4 kHz to 10 kHz	0.3	0.7
For > 10 kHz to 20 kHz	0.3	1.0
5. Frequency and time weightings at 1 kHz	0.2	0.2
6. Long - term stability	0.1	0.1
7. Level linearity on the reference level range	0.2	0.3
8. Level linearity including the level range control	0.2	0.3
9. Tone burst response	0.2	0.3
10. Peak C sound level	0.2	0.35
11. Overload indication	0.2	0.25
12. High level stability	0.1	0.1

g. Petch.

Cert. No. : ACL25101
Job No. : VC68AC0064
Page : 4 of 8

Result of calibration :

1. Absolute sensitivity

Reference Acoustic Signal (dB)	Measured Value (dB)	Deviation (dB)	Acceptance Limit (dB)
93.9 (93.94)	93.9	0.0	±0.3

2. Self-generated noise

2.1 Normal test

Measured Value (dB)
18.8

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Weighting (dB)
A - weight	16.3
C - weight	22.1
Flat	28.0

3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
125	0.4	0.4	0.4	± 1.5
1000	0.1	0.1	0.1	± 1.0
8000	-0.2	-0.2	-0.2	±5.0

S. Ketchum

Cert. No. : ACL25101
Job No. : VC68AC0064
Pages : 5 of 8

4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	0.0	-0.1	0.0	±2.0
125	0.0	0.1	0.0	±1.5
250	0.0	0.0	0.0	±1.5
500	0.0	0.1	0.0	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.1	0.1	±2.0
4000	0.0	0.1	0.0	±3.0
8000	0.0	0.1	0.1	±5.0

5. Frequency and time weightings at 1 kHz

5.1 Frequency weightings at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.2
C - weight	94.0	94.0	0.0	± 0.2
Flat	94.0	94.0	0.0	± 0.2

5.2 Time weighting at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	94.0	94.0	0.0	± 0.1
Slow	94.0	94.0	0.0	± 0.1
Leq	94.0	94.0	0.0	± 0.1

6. Long - term stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.1	0.1	± 0.3

T. Retan

Cert. No. : ACL25101
Job No. : VC68AC0064
Pages : 6 of 8

7. Level linearity on the reference level range

Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
137.0	137.0	0.0	± 1.1
136.0	136.0	0.0	± 1.1
135.0	135.0	0.0	± 1.1
134.0	134.0	0.0	± 1.1
133.0	133.0	0.0	± 1.1
132.0	132.0	0.0	± 1.1
131.0	131.0	0.0	± 1.1
129.0	129.0	0.0	± 1.1
124.0	124.0	0.0	± 1.1
119.0	119.1	0.1	± 1.1
114.0	114.0	0.0	± 1.1
109.0	109.0	0.0	± 1.1
104.0	104.0	0.0	± 1.1
99.0	99.0	0.0	± 1.1
94.0	94.0	0.0	± 1.1
89.0	89.0	0.0	± 1.1
84.0	84.0	0.0	± 1.1
79.0	79.0	0.0	± 1.1
74.0	74.0	0.0	± 1.1
69.0	69.0	0.0	± 1.1
64.0	64.0	0.0	± 1.1
59.0	59.0	0.0	± 1.1
54.0	54.0	0.0	± 1.1
49.0	49.0	0.0	± 1.1
44.0	44.0	0.0	± 1.1
39.0	39.0	0.0	± 1.1
34.0	34.0	0.0	± 1.1
30.0	29.9	-0.1	± 1.1
29.0	29.0	0.0	± 1.1
28.0	28.0	0.0	± 1.1
27.0	26.9	-0.1	± 1.1
26.0	26.0	0.0	± 1.1
25.0	24.9	-0.1	± 1.1

R. Petchum.

Cert. No. : ACL25101

Job No. : VC68AC0064

Pages : 7 of 8

8. Level linearity including the level range control

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
130	94.0	94.0	0.0	±1.1

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
130	29.0	28.9	-0.1	±1.1

9. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Cycle	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	0.25	1	108.0	108.0	0.0	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.1	0.1	±1.0
Slow	2	8	108.0	108.0	0.0	1.5 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
SEL	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.0	0.0	±1.0

T. Reith

Cert. No. : ACL25101
Job No. : VC68AC0064
Pages : 8 of 8

10. Peak C sound level

Number of cycle in test signal	Anticipated Value (dB)	Measured Value, L _{cpeak} (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	130.0	130.0	0.0	±3.0
One	133.4	133.4	0.0	±3.0

Number of cycle in test signal	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	±2.0
Positive half cycle	135.4	135.1	-0.3	±2.0
Negative half cycle	135.4	135.1	-0.3	±2.0

11. Overload indication

Measured value (dB)		Deviated Value (dB)	Acceptance Limits (dB)
Positive one-half cycle	Negative one-half cycle		
89.6	89.6	0.0	±1.5

12. High level stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	137.1	137.0	0.1	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor $k = 2$
or any value following calculation, providing a level of confidence of approximately 95 %

End of Calibration Certificate

[Signature]

Cert. No. : ACL25107
Job No. : VC68AC0064
Pages : 7 of 8

8. Level linearity including the level range control

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
130	94.0	94.0	0.0	±1.1

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
130	29.0	29.2	0.2	±1.1

9. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Cycle	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.0	0.0	±1.0
Slow	2	8	108.0	108.0	0.0	1.5 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
SEL	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.0	0.0	±1.0

T. Petcha

Cert. No. : ACL25107
Job No. : VC68AC0064
Pages : 8 of 8

10. Peak C sound level

Number of cycle in test signal	Anticipated Value (dB)	Measured Value, Lcpeak (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	130.0	130.0	0.0	±3.0
One	133.4	133.3	-0.1	±3.0

Number of cycle in test signal	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	±2.0
Positive half cycle	135.4	135.2	-0.2	±2.0
Negative half cycle	135.4	135.2	-0.2	±2.0

11. Overload indication

Measured value (dB)		Deviated Value (dB)	Acceptance Limits (dB)
Positive one-half cycle	Negative one-half cycle		
89.5	89.6	0.1	±1.5

12. High level stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor $k = 2$
or any value following calculation, providing a level of confidence of approximately 95 %

End of Calibration Certificate

J. Petch.

**Certificate of Calibration****Customer**

Name : ALS Laboratory Group Thailand Co., Ltd.

Certificate No : 25-SLM-113

Address : 104 Soi Phatthanakan 40, Phatthanakan Road, Suan Luang, Bangkok 10250

Request No : Req-2025-0603

Unit Under Calibration Details

Measurement item : Sound Level Meter

Microphone Class : 2

Manufacturer : RION

Microphone Model : UC-52

Model : NL-42

Microphone S/N : 172170

Serial Number : 01173609

Preamplifier Model : NH-24

ID : RYG_FS0388

Preamplifier S/N : 74021

Resolution : 0.1 dB

Instrument Status : Used

Calibration Environment and Details

Temperature : 23 °C ± 2 °C

Humidity : 50 %RH ± 20 %RH

Barometric Pressure : 1013 hPa ± 10 hPa

Received Date : 6 March 2025

Calibrated Date : 19 March 2025

Calibration Procedure : In-house method CP-SLM-01 based on IEC 61672-3 : 2013 Electroacoustics - Sound level meters - Part 3; Periodic tests

Location of Calibration : Lab Acoustic

REVIEW BY	
APPROVED BY	
NEXT CAL DATE	19/03/26

Reference Standard

Instrument	Brand	Model	SN.	Due calibration	Traceability
Standard Microphone	Brüel & Kjær	4192	2294985	25 June 2025	NIMT
Audio Generator	Svantek	Svan401	131	15 October 2025	WK Electric

NoteThe reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor $k = 2$, providing a level of confidence approximately 95 %.

Calibrated By :

Mr. Noppadon Luangart
Service Calibration Engineer

Approved By :

Mr. Pacit Mathavorn
Calibration Engineer Supervisor

Issue Date : 19 March 2025

Certificate No : 25-SLM-113

Request No : Req-2025-0603

1. Indication at the calibration check frequency

UUC Setting	Nominal	Before Adjust		After Adjust		UNCERTAINTY (± dB)	Acceptance Limit (± dB)	Result
FAST / A / 30-130	Level	UUC	ERR	UUC	ERR			
Calibrator Setting	(dB)	(dB)	(dB)	(dB)	(dB)			
1000 Hz 94 dB	94.06	94.0	-0.06	94.1	+0.04	0.20	0.30	Pass

Note : Absolute sensitivity was established by the use of Sound Calibrator Brand RION, Model NC-75, SN.35002736

2. Self-generated noise, Microphone installed

UUC Setting	Measured	UNCERTAINTY
FAST / 30-130		
UUC Weighting	(dB)	(± dB)
A	15.8	0.10

3. Self-generated noise, Microphone replaced by the electrical input signal device

UUC Setting	Measured	UNCERTAINTY
FAST / 30-130		
UUC Weighting	(dB)	(± dB)
A	12.4	0.10
C	16.7	0.10
Z	20.7	0.10

4. Acoustic signal test of frequency weightings (Without Windscreen)

UUC Setting	Deviation from various Frequency Weighting Responce curve			UNCERTAINTY (± dB)	Acceptance Limit (± dB)	Result
FAST / 30-130	A	C	Z			
STD Setting	(dB)	(dB)	(dB)	(± dB)	(± dB)	
125 Hz	0.2	0.4	0.4	0.60	1.5	Pass
1000 Hz	0.0	0.0	0.0	0.60	1.0	Pass
4000 Hz	-0.1	-0.1	-0.1	0.60	3.0	Pass
8000 Hz	-1.4	-1.4	-1.3	0.70	5.0	Pass1

Certificate No : 25-SLM-113

Request No : Req-2025-0603

5. Electrical signal test of frequency weightings, Weighting network response with relative to 1 kHz

UUC Setting	Deviation from various Frequency			UNCERTAINTY	Acceptance	Result
FAST / 30-130	Weighting Responce curve				Limit	
STD Setting	A (dB)	C (dB)	Z (dB)	(± dB)	(± dB)	
63 Hz	-0.2	-0.1	0.0	0.20	2.0	Pass
125 Hz	-0.1	0.0	0.0		1.5	Pass
250 Hz	-0.1	0.0	0.0		1.5	Pass
500 Hz	0.0	0.0	0.0		1.5	Pass
1000 Hz	0.0	0.0	0.0		1.0	Pass
2000 Hz	0.0	0.1	0.0		2.0	Pass
4000 Hz	0.0	0.0	0.0		3.0	Pass
8000 Hz	0.1	0.1	0.0		5.0	Pass
16000 Hz	-1.3	-1.4	0.0		+5, -INF.	Pass

6. Frequency and time weightings at 1kHz

UUC Setting	STD	Measured		UNCERTAINTY (± dB)	Acceptance	Result
FAST / 30-130	REF	UUC	ERR		Limit	
UUC Weighting	(dB)	(dB)	(dB)	(± dB)	(± dB)	
A	114.00	114.0	0.0	0.20	0.20	
C	114.00	114.0	0.0		0.20	
Z	114.00	114.0	0.0		0.20	

UUC Setting	STD	Measured		UNCERTAINTY (± dB)	Acceptance	Result
30-130 / A	REF	UUC	ERR		Limit	
UUC Time Response	(dB)	(dB)	(dB)	(± dB)	(± dB)	
Fast	114.00	114.0	0.0	0.20	0.10	
Slow	114.00	114.0	0.0		0.10	
Leq	114.00	114.0	0.0		0.10	

Certificate No : 25-SLM-113

Request No : Req-2025-0603

7. Long Term Stability

UUC Setting	Measured	UNCERTAINTY (± dB)	Acceptance Limit (± dB)	Result
FAST / A / 30-130	UUC			
STD Setting	(dB)			
Initial	114.0	0.10	0.30	Pass
Final	114.0			
Deviated	0.0			

8. Level linearity on the reference level range

UUC Setting	Anticipated	Deviation		UNCERTAINTY (± dB)	Acceptance Limit (± dB)	Result
FAST / A / 30-130	REF	UUC	ERR			
STD dB	(dB)	(dB)	(dB)			
138.00	138	137.9	-0.1	0.30	1.1	Pass
134.00	134	134.0	0.0		1.1	Pass
129.00	129	128.9	-0.1		1.1	Pass
124.00	124	124.0	0.0		1.1	Pass
119.00	119	119.0	0.0		1.1	Pass
114.00	114	114.0	0.0		1.1	Pass
109.00	109	109.0	0.0		1.1	Pass
104.00	104	104.0	0.0		1.1	Pass
99.00	99	99.0	0.0		1.1	Pass
94.00	94	94.0	0.0		1.1	Pass
89.00	89	89.0	0.0		1.1	Pass
84.00	84	84.0	0.0		1.1	Pass
79.00	79	79.0	0.0		1.1	Pass
74.00	74	74.0	0.0		1.1	Pass
69.00	69	69.0	0.0		1.1	Pass
64.00	64	64.0	0.0		1.1	Pass
59.00	59	59.0	0.0		1.1	Pass
54.00	54	54.0	0.0		1.1	Pass
49.00	49	49.0	0.0		1.1	Pass
44.00	44	44.0	0.0		1.1	Pass
39.00	39	39.0	0.0		1.1	Pass
34.00	34	34.0	0.0		1.1	Pass
29.00	29	29.0	0.0		1.1	Pass
24.00	24	24.1	0.1		1.1	Pass

Certificate No : 25-SLM-113

Request No : Req-2025-0603

9. Level linearity including the level range control

UUC Setting	STD	Measured		UNCERTAINTY	Acceptance	Result
FAST / A	REF	UUC	ERR	(± dB)	Limit	
UUC Range	(dB)	(dB)	(dB)		(± dB)	
30-130	29.50	29.6	0.1	0.30	1.1	Pass
	114	114.0	0.0		1.1	Pass

10. Tone burst response

UUC Setting	STD	Anticipated	Measured		UNCERTAINTY	Acceptance	Result
A / 30-130	Toneburst	Ref	UUC	ERR	(± dB)	Limit	
UUC Time Response	(ms)	(dB)	(dB)	(dB)		(± dB)	
Fast	200	126.0	126.0	0.0	0.20	1.0	Pass
	2	109.0	109.0	0.0		+1.0, -2.5	Pass
	0.25	100.0	99.9	-0.1		+1.5, -5.0	Pass
Slow	200	119.6	119.6	0.0		1.0	Pass
	2	100.0	100.0	0.0		+1.0, -5.0	Pass
SEL	200	120.0	120.0	0.0		1.0	Pass
	2	100.0	100.0	0.0		+1.0, -2.5	Pass
	0.25	91.0	90.9	-0.1		+1.5, -5.0	Pass

11. Peak C Sound level

UUC Setting	Anticipated	Measured		UNCERTAINTY	Acceptance	Result
FAST / C / 55-141	REF	UUC	ERR	(± dB)	Limit	
STD Setting	(dB)	(dB)	(dB)		(± dB)	
Complete cycle	136.4	136.4	0.00	0.20	3.0	Pass
Positive half cycle	135.4	135.2	-0.20		2.0	Pass
Negative half cycle	135.4	135.2	-0.20		2.0	Pass

Certificate No : 25-SLM-113

Request No : Req-2025-0603

12. Overload indication

UUC Setting	Measured	UNCERTAINTY (± dB)	Acceptance	Result
FAST / A / 30-130	UUC		Limit	
STD Setting	(dB)		(± dB)	
Positive one-half cycle	139.5			
Negative one-half cycle	139.4			
Deviated	0.1	0.20	1.5	Pass

13. High Level Stability

UUC Setting	Measured	UNCERTAINTY (± dB)	Acceptance	Result
FAST / A / 30-130	UUC		Limit	
STD Setting	(dB)		(± dB)	
Initial	129.0			
Final	129.0			
Deviated	0.0	0.10	0.30	Pass

Note :

Function	Maximum-permitted Uncertainty of measurement
1. Indication at the calibration check frequency	Not applicable
2. Self-generated noise, Microphone installed	Not applicable
3. Self-generated noise, Microphone replaced by the electrical input signal device	Not applicable
4. Acoustic signal test of frequency weightings at 10 Hz to 4 kHz	0.60 dB
4. Acoustic signal test of frequency weightings at >4 kHz to 10 kHz	0.70 dB
5. Electrical signal test of frequency weightings, Weighting network response with relative to 1 kHz	0.20 dB
6. Frequency and time weightings at 1kHz	0.20 dB
7. Long Term Stability	0.10 dB
8. Level linearity on the reference level range	0.30 dB
9. Level linearity including the level range control	0.30 dB
10. Tone burst response	0.30 dB
11. Peak C Sound level	0.35 dB
12. Overload indication	0.25 dB
13. High Level Stability	0.10 dB

- Acceptance limit and Maximum-permitted Uncertainty was IEC 61672-1:2013

Certificate No : 25-SLM-113

Request No : Req-2025-0603

Decision Rule for Statements of Conformity


The standard decision rule employed for the statements of conformity to each calibration result will be applied using ILAC-G8:09/2019; Guidelines on the Reporting of Compliance with Specification as following Fig. and statements

Pass = The measurement result plus the expanded uncertainty with a 95% coverage probability were within the limit.

Pass¹ = The measurement result was within the limit. However, a portion of the expanded uncertainty of measurement at 95% exceeds the limit.

Fail¹ = The measurement result was out of the limit. However, a portion of the expanded uncertainty of measurement at 95% is within the limit.

Fail = The measurement result plus the expanded uncertainty with a 95% coverage probability were outside the limit.

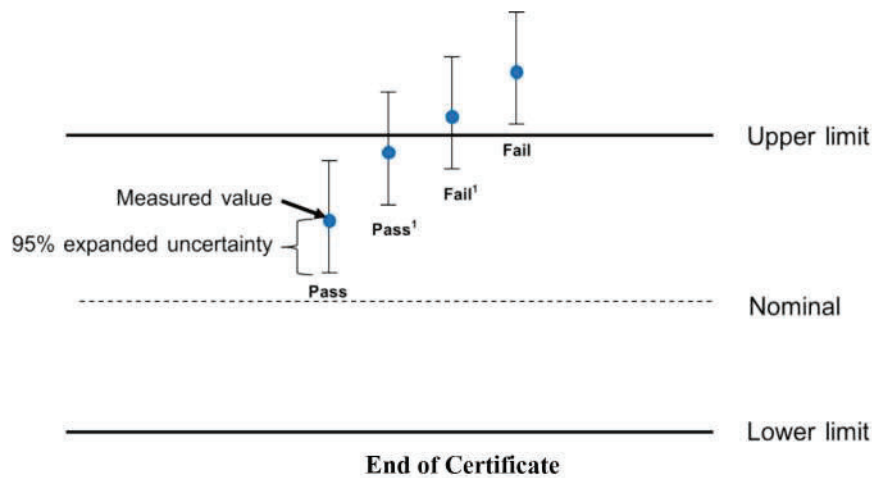

Certificate of Calibration

Customer



Name : ALS Laboratory Group Thailand Co., Ltd. **Certificate No** : 25-ACT-010
Address : 104 Soi Phatthanakan 40, Phatthanakan Road, Suan Luang, **Request No** : Req-2025-0091
Bangkok 10250

Unit Under Calibration Details

Measurement item : Acoustic Calibrator Class : 1
Manufacturer : RION Range : 94 dB / 1000 Hz
Model : NC-74 Instrument Status : Used
Serial Number : 34178121
ID : RYG_FS0213

Calibration Environment and Details

Temperature : (23 \pm 2 $^{\circ}$ C)
Humidity : (50 \pm 20 %RH)
Barometric Pressure : (1013 \pm 10.0 hPa)
Received Date : 15 January 2025
Calibration Date : 16 January 2025
Location of Calibration : LAB 1 Acoustic
Calibration Procedure : In-house method CP-ACT-02 based on IEC 60942:2017 Electroacoustics - Sound calibrators


REVIEW BY	
APPROVED BY	
NEXT CAL DATE	16/01/26


Reference Standard	Model	Serial Number	Traceable	Due Calibration
Sound Calibrator	SV 35A	58079	EEI	12 June 2025
THD Multimeter	2015	1047765	NIMT	16 January 2025

Traceability : This certificate provides traceability of measurement to recognized national standard, and to the realization of the international System of Units (SI).

Note

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor $k=2$, providing a level of confidence approximately 95 %.

Calibrated By : 
Mr. Noppadon Luangart
Service Calibration Engineer

Approved By : 
Mr. Pacit Mathavorn
Calibration Engineer Supervisor

Issue Date : 16 January 2025

Certificate No : 25-ACT-010

Request No : Req-2025-0091

Sound pressure level

Calibration Results : Without Adjustment

Calibration Range (dB)	Without Adjustment (dB)		Adjustment (dB)		Uncertainty (± dB)	Acceptance limit Class 1 (± dB)	Result
	Measured	Deviated value	Measured	Deviated value			
94 dB / 1000 Hz	94.11	0.11	-	-	0.13	0.25	Pass

Frequency of Sound pressure level

Calibration Range (Hz)	Without Adjustment		Adjustment		Uncertainty (± %)	Acceptance limit Class 1 (± %)	Result
	Measured (Hz)	Deviated	Measured (Hz)	Deviated			
94 dB / 1000 Hz	1000.00	0.00	-	-	0.01	0.70	Pass

Total Harmonic Distortion plus Noise of Sound pressure level (THD+N %)

Calibration Range (Hz)	Without Adjustment	Adjustment	Uncertainty (± %)	Acceptance limit Class 1 (± %)	Result
	Measured (%)	Measured (%)			
94 dB / 1000 Hz	1.21	-	0.40	2.5	Pass

Note :

Function	Maximum-permitted Uncertainty of measurement
Sound pressure level	0.15 dB
Frequency	0.20%
Total distortion+noise	0.50%

- Acceptance limit was IEC60942:2017 Class 1
- The calibration results exclude the calibrator pressure correction
- The calibration results exclude the microphone volume correction

Certificate No : 25-ACT-010

Request No : Req-2025-0091

Decision Rule for Statements of Conformity


The standard decision rule employed for the statements of conformity to each calibration result will be applied using ILAC-G8:09/2019; Guidelines on the Reporting of Compliance with Specification as following Fig. and statements

Pass = The measurement result plus the expanded uncertainty with a 95% coverage probability were within the limit.

Pass¹ = The measurement result was within the limit. However, a portion of the expanded uncertainty of measurement at 95% exceeds the limit.

Fail¹ = The measurement result was out of the limit. However, a portion of the expanded uncertainty of measurement at 95% is within the limit.

Fail = The measurement result plus the expanded uncertainty with a 95% coverage probability were outside the limit.

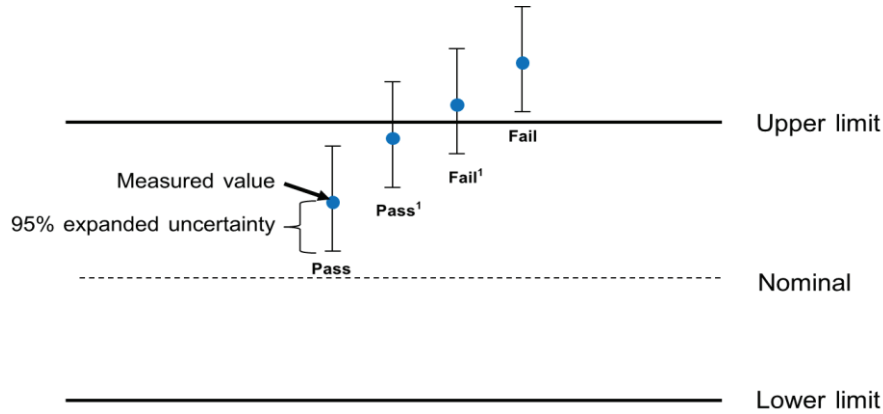

End of Calibration

Cert. No. : ACL25112

Pages : 1 of 8

Calibration Certificate

Equipment : SOUND LEVEL METER
Manufacturer : RION
Model : NL-42A / Microphone UC-52 / Preamplifier NH-24
Serial No.: 00623396 / 198643 / 26424
ID No.: RYG_FS0621

Condition As Found : GOOD

Customer : ALS LABORATORY GROUP (THAILAND) CO., LTD.
104 PHATTHANAKAN 40, PHATTHANAKAN ROAD,
KHWAENG PHATTHANAKAN, KHET SUAN LUANG,
BANGKOK, 10250 THAILAND.

Location : -
Ambient Temperature : (23.0 \pm 3) °C
Pressure : (101.3 \pm 3) kPa
Relative Humidity : (50.0 \pm 20) %

Received Date : 14 JANUARY 2025
Calibration Date : 27-29 JANUARY 2025
Date of Issue : 30 JANUARY 2025

REVIEW BY *Supt S*

APPROVED BY *[Signature]*

NEXT CAL DATE..... 26/ 01/ 2026

Calibrated by :

Nathakorn Pisutpaisan

Approved by :

T. Petchur
(Thanakul Petchurai)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

Cert. No. : ACL25112
Job No. : VC68AC0064
Pages : 2 of 8

Calibration Procedure : CP-AC-01

Calibration Method :

This equipment was calibrated by follow on IEC-61672-3 (2013) Standard for sound level meter (SLM).

The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.

For tests results of each items were made by observation of each Instruments display and also with SLM's display.

Condition of this result of calibration :

1. Reference Standard Instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
Waveform Generator	33210A	MY48017076	EF-0009-24	05-FEB-25
Waveform Generator	33511B	MY52302742	EF-0007-24	05-FEB-25
Digital Multimeter	33461A	MY53220104	EEL.BP 21/0267	13-FEB-25
Digital Multimeter	33461A	MY53220076	EEL.BP 20/0267	15-FEB-25
Digital Multimeter	34461A	MY60024273	EEL.BP 22/0267	15-FEB-25
Programmable Attenuator	MAT-1070	62100114	EF-0008-24	05-FEB-25
Condenser Microphone	4180	2977900	AA-1001-24	12-FEB-25
Measuring Amplifier	NA-42KAI	34560495	AA-3001-24	05-FEB-25

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is traceable to the international system of unit maintained at :

3.1 National Institute of Metrology (Thailand).

3.2 Thailand Institute of Scientific and Technological Research (TISTR).



Cert. No. : ACL25112
Job No. : VC68AC0064
Pages : 3 of 8

Summary of Measurement Result :

Parameter	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	0.2	N/A
2. Self-generated noise	0.2	N/A
3. Acoustical signal tests of frequency weightings		
125 Hz	0.3	0.6
1000 Hz	0.3	0.6
8000 Hz	0.3	0.7
4. Electrical signal tests of frequency weightings		
For 10 Hz to 4 kHz	0.3	0.6
For > 4 kHz to 10 kHz	0.3	0.7
For > 10 kHz to 20 kHz	0.3	1.0
5. Frequency and time weightings at 1 kHz	0.2	0.2
6. Long - term stability	0.1	0.1
7. Level linearity on the reference level range	0.2	0.3
8. Level linearity including the level range control	0.2	0.3
9. Tone burst response	0.2	0.3
10. Peak C sound level	0.2	0.35
11. Overload indication	0.2	0.25
12. High level stability	0.1	0.1

T. Retch.

Cert. No. : ACL25112
Job No. : VC68AC0064
Page : 4 of 8

Result of calibration :

1. Absolute sensitivity

Reference Acoustic Signal (dB)	Measured Value (dB)	Deviation (dB)	Acceptance Limit (dB)
93.9 (93.94)	93.9	0.0	±0.3

2. Self-generated noise

2.1 Normal test

Measured Value (dB)
14.8

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Weighting (dB)
A - weight	11.3
C - weight	18.9
Flat	24.4

3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
125	0.3	0.3	0.3	± 1.5
1000	0.1	0.1	0.1	± 1.0
8000	0.6	0.6	0.6	±5.0

T. Petch.

Cert. No. : ACL25112
Job No. : VC68AC0064
Pages : 5 of 8

4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	0.0	0.1	0.1	±2.0
125	0.1	0.1	0.1	±1.5
250	0.1	0.1	0.0	±1.5
500	0.0	0.1	0.0	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.1	0.0	±2.0
4000	0.0	0.0	0.0	±3.0
8000	0.0	0.1	0.1	±5.0

5. Frequency and time weightings at 1 kHz

5.1 Frequency weightings at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.2
C - weight	94.0	94.0	0.0	± 0.2
Flat	94.0	94.0	0.0	± 0.2

5.2 Time weighting at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	94.0	94.0	0.0	± 0.1
Slow	94.0	94.0	0.0	± 0.1
Leq	94.0	94.0	0.0	± 0.1

6. Long - term stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.1	0.1	± 0.3

T. Ketchum

Cert. No. : ACL25112
Job No. : VC68AC0064
Pages : 6 of 8

7. Level linearity on the reference level range

Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
137.0	137.0	0.0	± 1.1
136.0	136.0	0.0	± 1.1
135.0	135.0	0.0	± 1.1
134.0	134.0	0.0	± 1.1
133.0	133.0	0.0	± 1.1
132.0	132.0	0.0	± 1.1
131.0	131.0	0.0	± 1.1
129.0	129.0	0.0	± 1.1
124.0	124.0	0.0	± 1.1
119.0	119.0	0.0	± 1.1
114.0	114.0	0.0	± 1.1
109.0	109.0	0.0	± 1.1
104.0	104.0	0.0	± 1.1
99.0	99.0	0.0	± 1.1
94.0	94.0	0.0	± 1.1
89.0	89.0	0.0	± 1.1
84.0	84.0	0.0	± 1.1
79.0	79.0	0.0	± 1.1
74.0	74.0	0.0	± 1.1
69.0	69.0	0.0	± 1.1
64.0	64.0	0.0	± 1.1
59.0	59.0	0.0	± 1.1
54.0	54.0	0.0	± 1.1
49.0	49.0	0.0	± 1.1
44.0	44.0	0.0	± 1.1
39.0	39.0	0.0	± 1.1
34.0	34.0	0.0	± 1.1
30.0	30.1	0.1	± 1.1
29.0	29.0	0.0	± 1.1
28.0	28.1	0.1	± 1.1
27.0	27.1	0.1	± 1.1
26.0	26.2	0.2	± 1.1
25.0	25.1	0.1	± 1.1

T. Retoh.

Cert. No. : ACL25112
Job No. : VC68AC0064
Pages : 7 of 8

8. Level linearity including the level range control

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
130	94.0	94.0	0.0	±1.1

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
130	29.0	29.1	0.1	±1.1

9. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Cycle	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.1	0.1	±1.0
Slow	2	8	108.0	108.0	0.0	1.5 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
SEL	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.1	0.1	±1.0

T. Petch.

Cert. No. : ACL25112
Job No. : VC68AC0064
Pages : 8 of 8

10. Peak C sound level

Number of cycle in test signal	Anticipated Value (dB)	Measured Value, L _{cpeak} (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	130.0	130.0	0.0	±3.0
One	133.4	133.4	0.0	±3.0

Number of cycle in test signal	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	±2.0
Positive half cycle	135.4	135.1	-0.3	±2.0
Negative half cycle	135.4	135.1	-0.3	±2.0

11. Overload indication

Measured value (dB)		Deviated Value (dB)	Acceptance Limits (dB)
Positive one-half cycle	Negative one-half cycle		
89.6	89.6	0.0	±1.5

12. High level stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor $k = 2$
or any value following calculation, providing a level of confidence of approximately 95 %

End of Calibration Certificate

S. Retoh .

Cert. No. : ACL25102

Pages : 1 of 8

Calibration Certificate

Equipment : SOUND LEVEL METER
Manufacturer : RION
Model : NL-42 / Microphone UC-52 / Preamplifier NH-24
Serial No.: 00296515 / 179119 / 87526
ID No.: RYG_FS0432

Condition As Found : GOOD

Customer : ALS LABORATORY GROUP (THAILAND) CO., LTD.
104 PHATTHANAKAN 40, PHATTHANAKAN ROAD,
KHWAEANG PHATTHANAKAN, KHET SUAN LUANG,
BANGKOK, 10250 THAILAND.

Location : -
Ambient Temperature : (23.0 \pm 3) °C
Pressure : (101.3 \pm 3) kPa
Relative Humidity : (50.0 \pm 20) %

Received Date : 14 JANUARY 2025
Calibration Date : 27-29 JANUARY 2025
Date of Issue : 30 JANUARY 2025

REVIEW BY *Supt S*

APPROVED BY *[Signature]*

NEXT CAL DATE..... 26/ 01/ 2026

Calibrated by :

Nathakorn Pisutpaisan

Approved by :

[Signature]
(Thanakul Petchurai)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

Cert. No. : ACL25102
Job No. : VC68AC0064
Pages : 2 of 8

Calibration Procedure : CP-AC-01

Calibration Method :

This equipment was calibrated by follow on IEC-61672-3 (2013) Standard for sound level meter (SLM).

The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.

For tests results of each items were made by observation of each Instruments display and also with SLM's display.

Condition of this result of calibration :

1. Reference Standard Instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
Waveform Generator	33210A	MY48017076	EF-0009-24	05-FEB-25
Waveform Generator	33511B	MY52302742	EF-0007-24	05-FEB-25
Digital Multimeter	33461A	MY53220104	EEL.BP 21/0267	13-FEB-25
Digital Multimeter	33461A	MY53220076	EEL.BP 20/0267	15-FEB-25
Digital Multimeter	34461A	MY60024273	EEL.BP 22/0267	15-FEB-25
Programmable Attenuator	MAT-1070	62100114	EF-0008-24	05-FEB-25
Condenser Microphone	4180	2977900	AA-1001-24	12-FEB-25
Measuring Amplifier	NA-42KAI	34560495	AA-3001-24	05-FEB-25

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is traceable to the international system of unit maintained at :

3.1 National Institute of Metrology (Thailand).

3.2 Thailand Institute of Scientific and Technological Research (TISTR).

T. Petch

Cert. No. : ACL25102
Job No. : VC68AC0064
Pages : 3 of 8

Summary of Measurement Result :

Parameter	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	0.2	N/A
2. Self-generated noise	0.2	N/A
3. Acoustical signal tests of frequency weightings		
125 Hz	0.3	0.6
1000 Hz	0.3	0.6
8000 Hz	0.3	0.7
4. Electrical signal tests of frequency weightings		
For 10 Hz to 4 kHz	0.3	0.6
For > 4 kHz to 10 kHz	0.3	0.7
For > 10 kHz to 20 kHz	0.3	1.0
5. Frequency and time weightings at 1 kHz	0.2	0.2
6. Long - term stability	0.1	0.1
7. Level linearity on the reference level range	0.2	0.3
8. Level linearity including the level range control	0.2	0.3
9. Tone burst response	0.2	0.3
10. Peak C sound level	0.2	0.35
11. Overload indication	0.2	0.25
12. High level stability	0.1	0.1

S. Petch.

Cert. No. : ACL25102
Job No. : VC68AC0064
Page : 4 of 8

Result of calibration :

1. Absolute sensitivity

Reference Acoustic Signal (dB)	Measured Value (dB)	Deviation (dB)	Acceptance Limit (dB)
93.9 (93.94)	93.9	0.0	±0.3

2. Self-generated noise

2.1 Normal test

Measured Value (dB)
14.2

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Weighting (dB)
A - weight	10.8
C - weight	17.3
Flat	23.0

3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
125	0.2	0.2	0.2	± 1.5
1000	0.0	0.0	0.0	± 1.0
8000	0.2	0.2	0.2	±5.0

T. Ketch.

Cert. No. : ACL25102
Job No. : VC68AC0064
Pages : 5 of 8

4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	-0.1	-0.1	-0.1	±2.0
125	0.0	0.0	0.0	±1.5
250	0.0	0.0	0.0	±1.5
500	0.0	0.0	0.0	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.0	0.0	±2.0
4000	0.0	0.0	0.0	±3.0
8000	0.0	0.1	0.1	±5.0

5. Frequency and time weightings at 1 kHz

5.1 Frequency weightings at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.2
C - weight	94.0	94.0	0.0	± 0.2
Flat	94.0	94.0	0.0	± 0.2

5.2 Time weighting at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	94.0	94.0	0.0	± 0.1
Slow	94.0	94.0	0.0	± 0.1
Leq	94.0	94.0	0.0	± 0.1

6. Long - term stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.3

g. Reichen

Cert. No. : ACL25102

Job No. : VC68AC0064

Pages : 6 of 8

7. Level linearity on the reference level range

Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
137.0	137.0	0.0	± 1.1
136.0	136.0	0.0	± 1.1
135.0	135.0	0.0	± 1.1
134.0	134.0	0.0	± 1.1
133.0	133.0	0.0	± 1.1
132.0	132.0	0.0	± 1.1
131.0	131.0	0.0	± 1.1
129.0	129.0	0.0	± 1.1
124.0	124.0	0.0	± 1.1
119.0	119.0	0.0	± 1.1
114.0	114.0	0.0	± 1.1
109.0	109.0	0.0	± 1.1
104.0	104.0	0.0	± 1.1
99.0	99.0	0.0	± 1.1
94.0	94.0	0.0	± 1.1
89.0	89.0	0.0	± 1.1
84.0	84.0	0.0	± 1.1
79.0	79.0	0.0	± 1.1
74.0	74.0	0.0	± 1.1
69.0	69.0	0.0	± 1.1
64.0	64.0	0.0	± 1.1
59.0	59.0	0.0	± 1.1
54.0	53.9	-0.1	± 1.1
49.0	49.0	0.0	± 1.1
44.0	44.0	0.0	± 1.1
39.0	38.9	-0.1	± 1.1
34.0	33.9	-0.1	± 1.1
30.0	29.9	-0.1	± 1.1
29.0	28.9	-0.1	± 1.1
28.0	27.9	-0.1	± 1.1
27.0	26.9	-0.1	± 1.1
26.0	25.9	-0.1	± 1.1
25.0	24.9	-0.1	± 1.1

S. Petch.

Cert. No. : ACL25102
Job No. : VC68AC0064
Pages : 7 of 8

8. Level linearity including the level range control

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
130	94.0	94.0	0.0	±1.1

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
130	29.0	28.8	-0.2	±1.1

9. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Cycle	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.0	0.0	±1.0
Slow	2	8	108.0	108.0	0.0	1.5 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
SEL	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.0	0.0	±1.0

T. Petch.

Cert. No. : ACL25102
Job No. : VC68AC0064
Pages : 8 of 8

10. Peak C sound level

Number of cycle in test signal	Anticipated Value (dB)	Measured Value, L _{cpeak} (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	130.0	130.0	0.0	±3.0
One	133.4	133.3	-0.1	±3.0

Number of cycle in test signal	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	±2.0
Positive half cycle	135.4	135.2	-0.2	±2.0
Negative half cycle	135.4	135.2	-0.2	±2.0

11. Overload indication

Measured value (dB)		Deviated Value (dB)	Acceptance Limits (dB)
Positive one-half cycle	Negative one-half cycle		
89.5	89.5	0.0	±1.5

12. High level stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor $k = 2$
or any value following calculation, providing a level of confidence of approximately 95 %

End of Calibration Certificate

T. Petch.



JIRANATEE ASSOCIATES CO.,LTD.

Jiranatee Associates Co.,Ltd
63/14-15, 67/35-36
Petchkasem 7,7/1, Rd. Watthapra, Bangkokyai,
Bangkok 10600 (Thailand)
Tel: +6608680812
Mobile: +66863999453
E-mail: jnac-calibration@jiranatee.com
Web site: www.jiranatee.com

Accredited calibration laboratory
ISO/IEC 17025:2017
NSC-TISI-TIS 17025
CALIBRATION 0367

Temperature measurement laboratory
Calibration services department.



CERTIFICATE OF CALIBRATION

Certificate No. : CDT-085-67

Page 1 of 2 Pages

MEASUREMENT ITEM : Heat Stress Monitor
MANUFACTURER : Delta OHM
MODEL/TYPE : HD32.2
SERIAL NUMBER : 15030244
ID NUMBER : RYG_FS0236
CONDITION AS-RECEIVED : Used item
CUSTOMER : ALS laboratory group (thailand) Co., Ltd.
104 Phatthanakan 40, Phatthanakan Rd.,
Khwaeng Suan Luang, Khet Suan Luang,
Bangkok 10250 Thailand.

RECEIVED DATE : 15 May 2024
MEASUREMENT DATE : 17 May 2024
ISSUE DATE : 21 May 2024

ENVIRONMENTAL CONDITIONS:

Ambient condition in the laboratory are as follow:

Temperature : 23.0 ± 3.0 °C
Relative Humidity : 55.0 ± 15.0 %RH

NOTED: The certificate is valid only to the item calibrated on date and place of calibration.

TABULATION OF RESULTS:

The table on next page give the measured values.

Calibration procedure:

The temperature calibration was done by In-House calibration method as WI-CL-001 according to comparison method with standard digital temperature indicator and standard temperature probe. The temperature scale use was based on ITS-90.

Traceability:

The measurement results are traceable to the international system of units (SI) through National Institute of Metrology Thailand (NIMT) Certificate number: TT-0047-24, Certificate number: ER-0101-23

Reference Used During Calibration:

1. Standard Temperature Probe
Model: STS-100 A500, Serial No.: 667682-09,
Due date: 26 Mar 2025
2. Digital Temperature Indicator
Model: DTI-1000-A MK II, Serial No.: 671407-00591 Due date: 14 Sep 2024

Uncertainty of Measurement:

The reported uncertainty of measurement is based on the standard uncertainty multiplied by a coverage factor $k=2$, Which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty has been determined in accordance with the GUM 'Evaluation of measurement data - Guide to the expression of uncertainty in measurement'



Calibrated by:

- ☐ Mr. Sorawit Thachalad
☐ Miss Jittrapon Lertsomphol
☒ Miss Ruangrumpai Phoommit

Approved signatory:

Mr. Parinya Booncharoen
Calibration Department Manager

Result of Calibration: ☒ Without Adjustment ☐ With Adjustment

Calibration Range: 20 °C to 40 °C

Function:

Table 1: This equipment was connected with wet bulb probe Model: HP3201.2 S/N: 20030506.
Dimension: Diameter 3.3 mm. Length 170 mm.

<u>Immersion Depth</u> (mm)	<u>Standard Reading</u> (°C)	<u>UUC Reading</u> (°C)	<u>Error</u> (°C)	<u>Uncertainty</u> (°C)
80	20.058	20.1	0.0	0.099
80	25.047	25.1	0.1	0.099
80	30.042	30.1	0.1	0.099
80	35.035	35.1	0.1	0.099
80	40.025	40.1	0.1	0.099

Table 2: This equipment was connected with Globe thermometer probe Model: TP3276.2 S/N: 17009684.
Dimension: Diameter 3.3 mm. Length 205 mm.

<u>Immersion Depth</u> (mm)	<u>Standard Reading</u> (°C)	<u>UUC Reading</u> (°C)	<u>Error</u> (°C)	<u>Uncertainty</u> (°C)
110	20.058	20.0	-0.1	0.099
110	25.047	25.0	0.0	0.099
110	30.042	30.0	0.0	0.099
110	35.035	35.0	0.0	0.099
110	40.025	40.0	-0.1	0.16

Table 3: This equipment was connected with temperature probe Model: TP3207.2 S/N: 15033223.
Dimension: Diameter 14 mm. Length 150 mm.

<u>Immersion Depth</u> (mm)	<u>Standard Reading</u> (°C)	<u>UUC Reading</u> (°C)	<u>Error</u> (°C)	<u>Uncertainty</u> (°C)
75	20.059	20.1	0.0	0.099
75	25.047	25.0	0.0	0.099
75	30.043	29.8	-0.2	0.099
75	35.035	34.7	-0.3	0.099
75	40.024	39.6	-0.4	0.099

UUC*: Unit Under Calibration

Remark: The reported uncertainty of measurement is 0.16, based on standard uncertainty multiplied by a coverage factor k=2.21 providing a level of confidence of approximately 95%.

End of Certificate of Calibration





TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000-29 FAX. 0-2719-9484



Cert.No.: 24CH96
Page.: 1 of 3

Certificate of Calibration

Equipment : pH Meter
Manufacturer : Mettler Toledo
Model : SevenCompact S220
Serial No. : C104059460
ID No. : RYG_EN0183
Condition As-Received: Used Item
Received Date : 18 January 2024
Calibration Date : 19 January 2024
Reference : 2401-0579DSC-2
Submitted by : ALS Laboratory Group (Thailand) Co.,Ltd. (Rayong Branch)
616/10 Moo 5, T.Maenam Khu,
A.Pluakdaeng, Rayong 21140, Thailand

REVIEW BY	N. Banwit
APPROVED BY	[Signature]
NEXT CAL. DATE	19/01/25

1316174 ปลื้มจิตราภรณ์
Cd

Ambient Temperature : (25 ± 2.5) °C
Relative Humidity : (50 ± 15) %
Calibration Procedure : In - house method :
- CP-CH5 by direct measurement with standard voltage calibrator and direct measurement with certified reference material (CRM)
- CP-CH8 by comparison with temperature standard

Calibrated by : Warakorn Lernagatrakul

Approved by :

[Signature]

Approved Signatory

- (✓) Saithip Meangmai
() Warakorn Lernagatrakul
() Ponpan Paipim

Issue Date : 24 January 2024

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

A 0062854



Cert.No.: 24CH96

Page.: 2 of 3

Condition of this calibration result

1. Reference Standard Instrument

<u>Instrument</u>	<u>Serial No.</u>	<u>ID No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
1) Document Process Calibrator	54030049	130RC116	23E2802	27 Aug 2024
2) Ref. Standard Thermometer	4982054	110RC044	23I908	26 July 2024

This certification is traceable to the International System of Unit maintained through:-

- Technology Promotion Association (Thailand-Japan)

2. Certified Reference Materials : The measurement results are traceable to SI through CPA chem Ltd.,
ANSI-ASQ National Accreditation Board, Accredited No. AR-1835

<u>Buffer Solution</u>	<u>Manufacturer</u>	<u>Lot No.</u>	<u>Exp. date</u>
pH 4.008	CPA chem	940102	27 Nov 2025
pH 6.986	CPA chem	940104	02 Nov 2024
pH 9.997	CPA chem	940106	02 Nov 2024

3. This certificate is valid only to the item calibrated on date and place of calibration.

Calibration Results

Function : mV Measurement

Performing standard curve by Fluke at pH (4,7,10)

<u>Unit Under Calibration</u>	<u>Nominal Value</u>	<u>Standard Voltage Input</u>	<u>Actual Reading</u>		<u>Uncertainty of Measurement</u> (±mV)	<u>Coverage factor</u> <i>k</i>
	<u>pH</u>	<u>mV</u>	<u>mV</u>	<u>pH</u>		
pH Meter S/N.: C104059460	4.000	177.48	177.4	4.000	0.058	2.00
	7.000	0.00	0.0	7.000	0.058	2.00
	10.000	-177.48	-177.5	10.000	0.058	2.00

Saithip

a 1198287



Cert.No.: 24CH96
Page.: 3 of 3

Calibration Results

Function : pH Measurement

Performing three buffers standard curve by using buffer nominal pH (4.01,7.00,10.01)

Unit Under Calibration	Standard pH Buffer Solution	Actual pH Reading	Actual mV Reading (mV)	Uncertainty of pH Measurement (\pm)	Coverage factor k
pH Electrode S/N.: 3225367	4.008	4.013	176.0	0.0054	2.07
	6.986	6.983	2.2	0.0084	2.00
	9.997	9.996	-174.1	0.0065	2.00

Function : Temperature Measurement

(*) Without adjustment

This equipment was connected with Temperature Probe;

- Model : InLab®Expert Pro-ISM
- Serial No. : 3225367

Dimension of probe

- Length : 120 mm.
- Diameter : 12 mm.
- Immersion Depth : 100 mm.

Calibration Point (°C)	Standard Temperature (°C)	UUC* Reading (°C)	Error (°C)	Uncertainty of measurement (\pm °C)	Coverage factor k
25.0	25.001	25.2	0.199	0.13	2.00

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k , providing a level of confidence of approximately 95 %.

-o0o-

Saitip

a 1198288



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG, BANGKOK 10250
TEL. 0-2717-3000-24 FAX. 0-2719-9484



Certificate of Calibration

Certificate No. : 24E289

Page : 1 of 2

Equipment : pH Meter
Manufacturer: Mettler Toledo
Model : SevenCompact S220
Serial No.: C104059460
ID No.: RYG_EN0183

This certificate may not be reproduced other than in full,
except with the prior written approval of the head of
Corporate Services 3: Equipment Calibration and Testing Services.

Condition As-Received: Used Item
Received Date: 18 January 2024
Calibration Date: 23 January 2024

Reference: 2401-0579DSC
Ambient Temperature: (23 \pm 2) °C
Relative Humidity: (50 \pm 10) %
Submitted by: ALS Laboratory Group (Thailand) Co.,Ltd. (Rayong Branch)
616/10 Moo 5, T.Maenam Khu, A.Pluakdaeng,
Rayong 21140, Thailand

Procedure used: Calibration were conducted using calibration procedure No. CP-E17 According to EURAMET cg-15.

Condition of this result of calibration

1.Reference standards instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Certificate No.</u>	<u>Due Date</u>
1) Multi-Product Calibrator	5500A	6315011	E2U2300035	29 May 2024

2.This result of calibration was made on requested at the point specified by customer.


3.The certificate is valid only to the item calibrated on date and place of calibration.

4.This Certification is traceable to the International System of Unit maintained through:-

-NA Caltechnologies Co.,Ltd., ANAB Accredited No. Calibration AC-2658

Calibrated by : Wutchareeporn Wongchutikrane
Issue Date : 24 January 2024

Approved Signatory :


[] Phalinee Prabpaipal
[x] Nuntawat Khamchai
[] Pongsagorn Boonyaporn

B 0333296



Cert. No.: 24E289

Page.: 2 of 2

Result of calibration :- (*) Without adjustment () After adjustment

Function: DC voltage measurement

Range: 2000 mV

<u>Standard Value</u>	<u>UUC* Reading</u>	<u>Error</u>	<u>Uncertainty</u>
(mV)	(mV)	(mV)	($\pm \mu V$)
-200.0000	-200.0	0.0	68
-150.0000	-150.0	0.0	65
-100.0000	-100.0	0.0	63
-50.0000	-50.0	0.0	61
0.0000	0.0	0.0	58
50.0000	50.0	0.0	61
100.0000	99.9	-0.1	63
150.0000	149.9	-0.1	65
200.0000	199.9	-0.1	68

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k=2$, providing a level of confidence of approximately 95 %

UUC* = Unit Under Calibration.

-o0o-



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL.0-2717-3000-29 FAX.0-2719-9484



Certificate of Calibration

Cert. No.: 25LM10

Page.: 1 of 2

Equipment : DO Meter with Sensor

Manufacturer : YSI

Model : 5000-115V

Serial No. : 15E102796

ID No. : RYG_EN0032

Submitted by : ALS Laboratory Group (Thailand) Co.,Ltd.
(Rayong Branch)
616/10 Moo 5 T. Maenam Khu, A. Pluakdaeng,
Rayong 21140 Thailand

Location : TPA On Site Calibration Laboratory

Received Order : 17 January 2025

Calibrated Date : 20 January 2025

Ambient Temperature : (26 ± 10) °C

Relative Humidity : (50 ± 30) %

AC Line Voltage : (220 ± 22) V

Calibrated by : Warakorn Lerngagtrakul

Approved by :

Approved Signatory

() Chakrit Waewwanjua

(✓) Suwit Imjai

() Kunchit Promprat

Issue Date : 23 January 2025

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

REVIEW BY Photchana S.

APPROVED BY

NEXT CAL DATE 20/07/26



Equipment : DO Meter with Sensor
Condition As-Received : Used Item
Reference : 2501-0600DSC-2

Cert. No.: 25LM10
Page.: 2 of 2

Procedure Used :-

Calibration were conducted using in-house calibration procedure CP-OT01 according to comparison with Industrial Platinum Resistance Thermometer (IPRT) into Temperature Bath.

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

<u>Instrument</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Traceable</u>	<u>Due Date</u>
1) Digital Thermometer	2188080	2411022	TPA	17 Sep 2025

2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certification is traceable to the International System of Unit.

Remark : TPA : Technology Promotion Association (Thailand - Japan)

Result of Calibration :- (*) Without Adjustment

Function : Temperature measurement.

This instrument was connected with temperature sensor, S/N.: 15E100464

<u>Calibration Point</u> (°C)	<u>Immersion Depth</u> (mm)	<u>Standard Temperature</u> (°C)	<u>UUC* Reading</u> (°C)	<u>Error</u> (°C)	<u>Uncertainty</u> (± °C)	<u>Coverage Factor</u> <i>k</i>
20.00	60	20.002	19.81	-0.192	0.15	2.00

UUC* : Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3 : EQUIPMENT CALIBRATION AND TESTING SERVICES


534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250

TEL. 0-2717-3000 FAX. 0-2719-9484

Certificate of Testing

Cert.No.: 25TW15

Page.: 1 of 2

Equipment :	DO Meter
Manufacturer :	YSI
Model :	5000-115V
Serial No. :	15E102796
ID No. :	RYG_EN0032
Received Date :	17 January 2025
Test Date :	20 January 2025
Reference :	2501-0600DSC-1
Submitted by :	ALS Laboratory Group (Thailand) Co.,Ltd. (Rayong Branch) 616/10 Moo 5, T.Maenam Khu, A.Pluakdaeng, Rayong 21140, Thailand
Laboratory Condition :	Temperature (25 ± 5) °C Humidity (50 ± 20) %
Test Procedure :	In - house method : CP-CH9 by Comparison Technique with Azide Modification Method
Tested by :	Walalak Sirithean
Approved by :	 _____ Approved Signatory
() Pornthippa Tameyakul () Ponpan Paipim (✓) Saithip Meangmai	
Issue Date :	21 January 2025



Cert.No.: 25TW15

Page.: 2 of 2

Condition of this result of calibration

1. Reference Standard Instruments :

This certification is traceable to the International System of Unit through the reference standards laboratory of Industrial Calibration Center, Technology Promotion Association (Thailand-Japan).

<u>Instruments</u>	<u>Serial No.</u>	<u>ID No.</u>	<u>Certificate No.</u>	<u>Due Date</u>
1. Burette	-	130BU10	23CG1172	22 Mar 2025
2. Balance	14233821	110RC001	24MM131	04 July 2025

2. Standard Material :-

<u>Material</u>	<u>Manufacturer</u>	<u>Lot.No.</u>	<u>Assay</u>
Sodium Thiosulfate 5-Hydrate AR	KEMAUS	2203162447	99.6%

Result : Dissolved Oxygen Meter Adjustment With Air 100 %

Dissolved Oxygen Probe No.: 15E100464

Titration Method (Azide Modification Method) (mg/L)	DO Meter Reading (mg/L)	Standard Deviation (mg/L)
8.20	8.20	0.0084

This report was certified only for the instrument we tested. It is allowable to use for study. Intend to use for advertising and referral purpose is prohibited. This report may not be reproduced other in full, without written approval of the laboratory

-o0o-



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL.0-2717-3000-29 FAX.0-2719-9484



Certificate of Calibration

Cert. No.: 24TM1663

Page : 1 of 3

Equipment : Low Temp. Incubator

Manufacturer : Memmert

Model : IPP750

Serial No. : V818.0084

ID No. : RYG_EN0154

Submitted by : ALS Laboratory Group (Thailand) Co.,Ltd. Rayong Branch
616/10 Moo 5, T.Maenam Khu,
A.Pluakdaeng,
Rayong 21140, Thailand

Location : BOD Room

Received Order : 01 November 2024

Calibration Date : 01 November 2024

Ambient Temperature : (26 ± 10) °C

Relative Humidity : (50 ± 30) %

AC Line Voltage : (220 ± 22) V

Calibrated by : Krisda Malee

Approved by :

Kunchit

Approved Signatory

() Ponpan Paipim

() Suwit Imjai

(✓) Kunchit Promprat

Issue Date :

07 November 2024

REVIEW BY *Thanitak*

APPROVED BY *D. Kunchit*

NEXT CAL DATE..... 01/05/26

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.



Equipment : Low Temp. Incubator
Condition As-Received : Used Item
Reference : 2411-0002OC-1

Cert. No.: 24TM1663

Page : 2 of 3

Procedure Used :-

Calibration were conducted using calibration procedure CP-OT02 based on TLAS G-20 according to direct measurement method with Data Acquisition which connected with Resistance Temperature Detector (RTD).

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

<u>Instrument</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Traceable</u>	<u>Due Date</u>
1) Data Acquisition	MY44073381	24LM73	TPA	18 May 2025

2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certification is traceable to the International System of Unit.


Remark : TPA : Technology Promotion Association (Thailand - Japan)

Result of Calibration :- (*) Without Adjustment

Function of UUC* : Temperature Source

Fresh air setting : Close

Environment during calibration		
	Beginning	Finished
Temp. (°C)	24	25
REL.Humid. (%)	55	53
AC Supply (Volt)	220	221

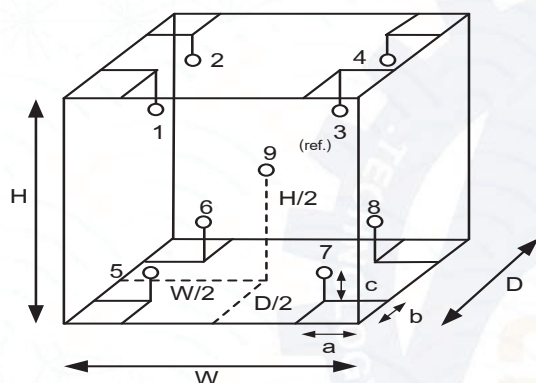

Position :	Ref. Std. ID No.:
1	1RTD-2/1
2	1RTD-2/2
3	22-01RTD-03
4	1RTD-2/4
5	1RTD-2/5
6	1RTD-2/6
7	23-01RTD-07
8	1RTD-2/8
9 (ref.)	23-01RTD-09

Probe Installation Details :

a = 10 cm
b = 10 cm
c = 10 cm

Dimension of Chamber :

D = 0.60 m
W = 1.0 m
H = 1.2 m
Capacity = 0.72 m³



Equipment : Low Temp. Incubator
Condition As-Received : Used Item
Reference : 2411-0002OC-1
Result of Calibration :- (*) Without Adjustment
Function of UUC* : Temperature Source
Fresh air setting : Close

Cert. No.: 24TM1663

Page : 3 of 3

Calibration Point (°C)	UUC* Setting (°C)	UUC* Reading (°C)	Temperature stability (± °C)	Temperature uniformity (°C)	Overall Variation (°C)	Coverage Factor <i>k</i>
20.0	20.0	20.0	0.026	0.26	0.53	2

Calibration Point (°C)	Measured Temperature (°C)									Uncertainty (±°C)
	Position									
	1	2	3	4	5	6	7	8	9 (ref.)	
20.0	20.071	19.915	20.273	20.179	19.977	19.782	20.056	20.026	20.033	0.30

Average* : The average of 30 values in each position.

Temperature stability : One-half of the greatest maximum difference of measured temperature at any one sensor.

Temperature uniformity : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.

Overall Variation : The Difference of the maximum and minimum measured temperatures throughout observation.

UUC* : Unit Under Calibration

Note : The reported uncertainty of measurement was included stability and excluded uniformity .

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-



Certificate of Calibration

Cert.No.: 24CG3711

Page.: 1 of 2

Equipment :	Burette
Capacity :	50 mL
Serial No. :	-
ID. No. :	RYG_EN0216
Manufacturer :	Witeg
Made in :	Germany
Submitted by :	ALS Laboratory Group (Thailand) Co.,Ltd. Rayong Branch 616/10 Moo 5, T.Maenam Khu, A.Pluakdaeng Rayong 21140, Thailand
Ambient Temperature :	(20 ± 2.5) °C
Relative Humidity :	(50 ± 10) %
Barometric Pressure :	756 mmHg
Calibration Procedure :	ASTM E 542 - 01
Calibrated by :	Sa-ngeunkam Wongsai

REVIEW BY *Thanitak.*

APPROVED BY *D. Johnson.*

NEXT CAL DATE *24/09/25*

Approved by :

Suda
Approved Signatory

(✓) Srisuda Khamtha
() Ponpan Paipim
() Unnophol Harachai

Issue Date :

24 September 2024

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.



Equipment : Burette
Received Date : 19 September 2024
Condition As-Received : Used Item
Calibration Date : 24 September 2024
Reference : 2409-0756DSC-3

Cert.No.: 24CG3711
Page.: 2 of 2

Condition of this result of calibration

1. Reference Standard Instruments :

<u>Instruments</u>	<u>Model</u>	<u>Serial No.</u>	<u>ID. No.</u>	<u>Certificate No.</u>	<u>Traceability</u>	<u>Due date</u>
1) Balance	XP205	B134206712	140RC007	24MM316	TPA	15 July 2025
2) Data Logger	HL-20D	20683159	140EC012	23H2174	TPA	10 Oct 2024
3) Thermometer	-	1594592	140EC010	24I175	TPA	20 Feb 2025

This certification is traceable to SI Unit

2. The certificate is valid only to the item calibrated on date and place of calibration.
3. True value is converted to true volume at the standard temperature of 20 °C


Calibration result :

Nominal capacity (mL)	Reading (mL)	Uncertainty (± mL)	k Factor
10	10.0259	0.0082	2.00
20	20.0214	0.0085	2.00
30	30.0006	0.0089	2.00
40	40.0003	0.0094	2.00
50	49.9988	0.011	2.00

Remark mL = cm³

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k* , providing a level of confidence of approximately 95 %.

-o0o-

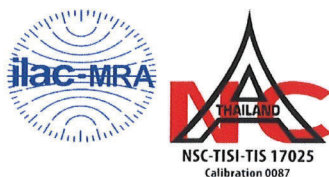


Certificate of Calibration

Equipment: SPECTROPHOTOMETER
Model: DR6000
Serial No. (or ID.): 1627845 (RYG_EN0037)
Manufacturer: HACH
Condition: In Condition

Certificate No.: C06250108
Issued Date: 18 March 2025
Job No.: WO-00064379
Page: 1 of 3

Customer: ALS Laboratory Group (Thailand) Co.,Ltd. (Rayong Branch)
616/10 Moo 5 T.Maenam Khu,
A.Pluakdaeng, Rayong 21140, Thailand.

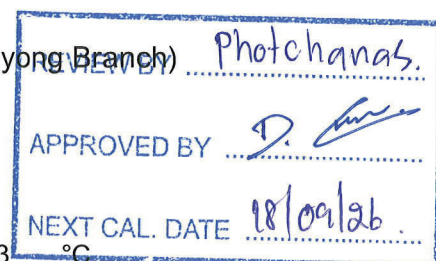

Environment Condition:

Temperature	24.4	°C	±	0.3	°C
Humidity	60.8	%RH	±	3.5	%RH

Calibration Place: ALS Laboratory Group (Thailand) Co.,Ltd. (Rayong Branch)
(Wet Chemistry Lab)
616/10 Moo 5 T.Maenam Khu, A.Pluakdaeng, Rayong 21140, Thailand.

Calibration By: Mr.Preecha Phooarsai

Calibration Date: 18 March 2025

The Method used: In house method, CAL-WI-24, base on ASTM E 275-08 and ASTM E 387-04


Traceability: This certificate is traceable to the CRM maintained by National Institute of Standards and Technology (NIST) through Starna Scientific Limited.

The standard for Wavelength Certificate No. 111583 and 111584

The standard for Photometric Certificate No. 9114984 and 111588

The standard for Stray light Certificate No. 111586 and 111585

The standard for Spectral resolution Certificate No. 111587



(Mr. Preecha Phooarsai)

Person in charge



(Miss Kaewkan Suradech)

Authorized signatory

This certificate is issued the units of measurement according to the International System of Units (SI). It provides traceability of measurement to international or national standard or other recognized national standard laboratories.

The measurement uncertainty stated is the expanded uncertainty which is obtained from the standard uncertainty multiplied by the coverage factor (k=2) to provide a level of confidence of approximately 95%. It is determined in accordance with the Guide to Expression of Uncertainty in Measurement (GUM).

These results may be affected by deviations from specified conditions. The results relate only to the items tested, calibrated or sampled. The report shall not be reproduced except in full without approval of DKSH Technology Limited.

บริษัท ดีเคเอสเอช เทคโนโลยี จำกัด
DKSH Technology Limited

2533 ถนนสุขุมวิท แขวงบางจาก เขตพระโขนง กรุงเทพมหานคร 10260
2533 Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260

Phone: +66 2639 7000 Email: info.calibration@dksh.com Website: www.dksh.com/scientific-thailand

Calibration Results:
Without Adjustment

Wavelength Accuracy (nm), The spectral bandwidth of Std at 2 nm and UUC at 2 nm

Standard Wavelength	Unit Under Calibration	Correction	Uncertainty
418.61	418.5	0.11	0.13
536.66	536.7	-0.04	0.13
637.98	638.3	-0.32	0.13
748.48	748.8	-0.32	0.13
807.03	807.5	-0.47	0.13

Photometric Accuracy (Absorbance)

Wavelength	Standard absorbance	Unit Under Calibration	Correction	Uncertainty
420 nm	0.0000	0.000	0.0000	0.0045
	0.2930	0.291	0.0020	0.0045
	0.5168	0.518	-0.0012	0.0045
	1.0298	1.031	-0.0012	0.0045
440 nm	0.0000	0.000	0.0000	0.0045
	0.2867	0.285	0.0017	0.0045
	0.5073	0.508	-0.0007	0.0045
	1.0083	1.009	-0.0007	0.0045
465 nm	0.0000	0.000	0.0000	0.0045
	0.2516	0.250	0.0016	0.0045
	0.4595	0.461	-0.0015	0.0045
	0.9334	0.935	-0.0016	0.0045
546.1 nm	0.0000	0.000	0.0000	0.0045
	0.2461	0.246	0.0001	0.0045
	0.4652	0.466	-0.0008	0.0045
	0.9468	0.948	-0.0012	0.0045
590 nm	0.0000	0.000	0.0000	0.0045
	0.2594	0.259	0.0004	0.0045
	0.5040	0.505	-0.0010	0.0045
	1.0032	1.004	-0.0008	0.0045
635 nm	0.0000	0.000	0.0000	0.0045
	0.2579	0.258	-0.0001	0.0045
	0.4971	0.497	0.0001	0.0045
	0.9720	0.973	-0.0010	0.0045

Calibration Results:
Without Adjustment
Photometric Accuracy (Absorbance)

Wavelength	Standard absorbance	Unit Under Calibration	Correction	Uncertainty
235 nm	0.0000	0.000	0.0000	0.0080
	0.7355	0.738	-0.0025	0.0080
257 nm	0.0000	0.000	0.0000	0.0080
	0.8574	0.857	0.0004	0.0080
313 nm	0.0000	0.000	0.0000	0.0080
	0.2864	0.290	-0.0036	0.0080
350 nm	0.0000	0.000	0.0000	0.0080
	0.6374	0.637	0.0004	0.0080

Stray light *

Standard: cut-off	UUC: Wavelength (nm)	UUC: Transmission (%T)	Absorbance (A)
260.62 +/- 0.11 nm	260.6	1.7	1.770
391.44 +/- 0.11 nm	391.4	1.4	1.854

Spectral Resolution *

Nominal Concentration 0.02 % v/v	Peak	Trough	Ratio	SBW
Standard Wavelength (nm)	268.66	266.69	1.38	2.00
UUC: Wavelength (nm)	268.2	266.2		
Std Absorbance (A)	0.4566	0.2780		
UUC: Absorbance (A)	0.413	0.299		

* Calibration Marked " Not TISI Accredited " in this Certificate have been included for completeness.

The End of Certificate

ใบตรวจสอบสภาพเครื่องวัดสิ่งแวดล้อม

เลขที่ใบงาน: WO-00064379

ชนิดเครื่องมือ: SPECTROPHOTOMETER

รุ่น: DR6000

หมายเลขเครื่อง: 1627845

ตรวจสอบ (รับ)		รายการตรวจเช็ค	ตรวจสอบ (ส่ง)		หมายเหตุ
18 Mar 2025			18 Mar 2025		
ปกติ	ไม่ปกติ		ปกติ	ไม่ปกติ	
		General			
<input checked="" type="checkbox"/>	<input type="checkbox"/>	1. ความสมบูรณ์เครื่อง	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	2. ความสะอาด (ช่องใส่ตัวอย่าง, ภายใน-นอกเครื่อง)	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	3. สวิทช์ ปิด – เปิด เครื่อง (On-Off Swicth)	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	4. ปุ่มกด (Keypad)	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	5. หน้าจอ (Display, Screen Contrast)	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
		Spectrophotometer			
<input type="checkbox"/>	<input type="checkbox"/>	6. แรงดันไฟฟ้า (Battery Backup) >= 2.5 VDC	<input type="checkbox"/>	<input type="checkbox"/>	
<input type="checkbox"/>	<input type="checkbox"/>	7. ตัวหมุนเลือกความยาวคลื่น (Wavelength Control)	<input type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	8. ความยาวคลื่น (Wavelength Check)	<input checked="" type="checkbox"/>	<input type="checkbox"/>	*
<input checked="" type="checkbox"/>	<input type="checkbox"/>	9. แหล่งกำเนิดแสง (UV < 3,000 hour)	<input checked="" type="checkbox"/>	<input type="checkbox"/>	13.5 Hours
<input checked="" type="checkbox"/>	<input type="checkbox"/>	10. แหล่งกำเนิดแสง (Visible < 5,000 hour)	<input checked="" type="checkbox"/>	<input type="checkbox"/>	893.0 Hours
<input checked="" type="checkbox"/>	<input type="checkbox"/>	11. ช่องวัดหลายตัวอย่าง (Carousel Module)	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
		pH Meter and Conductivity Meter			
<input type="checkbox"/>	<input type="checkbox"/>	12. อิเล็กโทรด (Electrode and Connection Cable)	<input type="checkbox"/>	<input type="checkbox"/>	
<input type="checkbox"/>	<input type="checkbox"/>	13. ระดับสารละลายใน Electrode (Level KCl)	<input type="checkbox"/>	<input type="checkbox"/>	
<input type="checkbox"/>	<input type="checkbox"/>	14. ฝาปิดกันปลาย Electrode (Dust Protection Hood)	<input type="checkbox"/>	<input type="checkbox"/>	
<input type="checkbox"/>	<input type="checkbox"/>	15. ขาจับอิเล็กโทรด (Stand)	<input type="checkbox"/>	<input type="checkbox"/>	
		Turbidimeter			
<input type="checkbox"/>	<input type="checkbox"/>	16. ค่าความขุ่นที่ต่ำสุด (No Sample)	<input type="checkbox"/>	<input type="checkbox"/>	
<input type="checkbox"/>	<input type="checkbox"/>	17. ระดับการส่องสว่างของแสง (>= 2.5 ไม่เกิน 3.0)	<input type="checkbox"/>	<input type="checkbox"/>	
		Automatic titrator			
<input type="checkbox"/>	<input type="checkbox"/>	18. สภาพ Piston Burettes	<input type="checkbox"/>	<input type="checkbox"/>	
<input type="checkbox"/>	<input type="checkbox"/>	19. Function Rinsing and Dosing	<input type="checkbox"/>	<input type="checkbox"/>	
<input type="checkbox"/>	<input type="checkbox"/>	20. ระบบท่อสายยางและอุปกรณ์ประกอบ	<input type="checkbox"/>	<input type="checkbox"/>	

เพิ่มเติม/ข้อแนะนำ : * 656.1nm = 656.1nm

* 486.0nm = 485.7nm

Mr.Preecha Phooarsai

Service Engineer

Accredited by

NSC-TISI-TIS 17025

Calibration 0426



Calibration certificate

Calibration Certificate No. 25BKL0004

Object	Electronic non-automatic weighing instrument	This calibration certificate documents the traceability to national standards.
Manufacturer	Sartorius	Uncertainties of measurements are taken into account when only statements of compliance are made.
Type	MSE224S-100-DU	This certificate was prepared by Sartorius Corporation in accordance to the current ISO/IEC 17025:2017 standard and Sartorius Work Instruction (Method) SOP WI 08.
Serial QM Ident. no.	26207038 RYG_EN0002	This certificate relate and apply this equipment only.
Customer	ALS Laboratory Group (Thailand) Co.,Ltd. (Rayong Branch)	
	616/10 Moo 5 T.Maenam Khu, A.Pluak Daeng, Rayong 21140, Thailand.	
Order no.	2230	
Number of pages	4	
Date of calibration	20 Feb 2025	

REVIEW BY *Thanita K.*APPROVED BY *D. Khunon.*

NEXT CAL DATE.....20/02/26

This calibration certificate may not be reproduced other than in full except with the permission of NSC-TISI-TIS-17025 and the issuing laboratory. Calibration certificates without signature are not valid.

The user is obliged to have the object recalibrated at appropriate intervals.

Date	06 Mar 2025	Approval of the Calibration Certificate	Person in charge
		Mr. Chonchai Inthana	Kachen Lalee

Calibration object

Single range instrument

Model	MSE224S-100-DU
Serial Number	26207038
QM Ident. no Inventory no.	RYG_EN0002 ---

Maximum capacity (Max. load)	220.0000 g
Measured range	220.0000 g
Scale interval	0.0001 g

Place of calibration

Address	According to page 1
Department Cost center	Laboratory Department. ---
Building Floor	--- 1st Floor.
Room	Balance Room.
Maximum temperature variation at place of calibration	5 K

Calibration procedure

EURAMET cg-18, V4.0 - Guidelines on the Calibration of Non-Automatic Weighing Instruments

Test equipment

Test equipment type	Test equipment ID	Valid until
Thermometer	MHB-382SD s/nB011342 Traceable to SI unit through DKSH	21 Aug 2025
Test weight set OIML R111 E2	Certificate No.M2308197S ,E2(Traceable to SI unit through TCS)	23 Aug 2025

Adjustment Status

The measuring device was internally adjusted before the calibration.

Environmental and measuring conditions

Date of calibration	20 Feb 2025
Temperature at place of calibration Temp. diff. <i>T</i> _{weights} - <i>T</i> _{place}	24.4 °C 0.6 K
Measuring conditions	The installation site is suitable. The device was levelled. Balance was loaded up to Max before test.
Comments	Humidity 50.2 %RH.

Measurement results | Measurement uncertainties

Repeatability

Test load (nominal): 10 g 200 g		
	10 g	200 g
1	10.0000 g	200.0000 g
2	10.0000 g	200.0001 g
3	10.0001 g	200.0001 g
4	10.0000 g	200.0000 g
5	10.0001 g	200.0000 g
6	10.0001 g	200.0001 g
7	10.0000 g	200.0000 g
8	10.0000 g	200.0001 g
9	10.0001 g	200.0000 g
10	10.0000 g	200.0000 g
	<i>s</i> = 0.00005 g	<i>s</i> = 0.00005 g

Eccentricity

Test load (nominal): 100 g	
Center	100.0000 g
Front left	99.9998 g
Back left	100.0000 g
Back right	100.0000 g
Front right	100.0000 g
Maximum deviation from centric loading indication $ \Delta_{ecc} _{max} = 0.0002\text{ g}$	

Error of indication

Testload	Indication	Error	Expansion factor	Uncertainty	Uncertainty relative
<i>L</i>	<i>I</i>	<i>E</i>	<i>k</i>	<i>U</i> (<i>E</i>)	<i>U</i> _{rel} (<i>E</i>)
0.0100 g	0.0100 g	0.0000 g	2.00	0.00013 g	1.3 %
0.1000 g	0.1000 g	0.0000 g	2.00	0.00013 g	0.13 %
0.5000 g	0.5000 g	0.0000 g	2.00	0.00013 g	0.027 %
1.0000 g	1.0000 g	0.0000 g	2.00	0.00013 g	0.013 %
5.0000 g	5.0000 g	0.0000 g	2.00	0.00014 g	0.0027 %
10.0000 g	10.0000 g	0.0000 g	2.00	0.00014 g	0.0014 %
20.0000 g	20.0000 g	0.0000 g	2.00	0.00014 g	0.00072 %
50.0000 g	50.0000 g	0.0000 g	2.00	0.00016 g	0.00032 %
100.0000 g	100.0001 g	0.0001 g	2.00	0.00021 g	0.00021 %
200.0000 g	200.0000 g	0.0000 g	2.00	0.00034 g	0.00017 %
220.0000 g	220.0000 g	0.0000 g	2.00	0.00039 g	0.00018 %
Maximum error of indication		$ E _{max} = 0.0001\text{ g}$			

*U*_{rel}(*E*) is the quotient of *U*(*E*) and test load *L*. The uncertainty of measurement *U*(*E*) is valid only if error *E* is considered. You will find reference notes on the uncertainty of measurement in use under: Appendix to the calibration certificate | Interpretation of measurement results.
Reference note: The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the documented Expansion factor, determined in accordance with the European Calibration Guideline EURAMET cg-18, V4.0. There is a 95 % probability that the value of the measurand will be in the assigned value range.

End of calibration certificate

Uncertainty of measurement in use

Device adjusted before measurement	Yes
Temperature deviation considered	1.5 K (isoCAL active)
Temperature coefficient considered	$1 \cdot 10^{-6}/\text{K}$


Uncertainty of the weighing result $U_{gl}(W)$

$U_{gl}(W) = 0.00013 \text{ g} + 3.95 \cdot 10^{-6} \cdot R$

Reference note: The current uncertainty of measurement is calculated by entering of the reading R into this formula. In relation to this, there is no need for a correction of the indication error. The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied with an Expansion factor of 2, determined in accordance with the European Calibration Guideline EURAMET cg-18, V4.0. There is a 95 % probability that the value of the measurand will be in the assigned value range.

Indication in % from max load	Net indication R	Uncertainty $U_{gl}(W)$	Uncertainty relative $U_{gl}(W)_{rel}$
1 %	2.2000 g	0.00014 g	0.0063 %
25 %	55.0000 g	0.00035 g	0.00063 %
50 %	110.0000 g	0.00056 g	0.00051 %
75 %	165.0000 g	0.00078 g	0.00047 %
100 %	220.0000 g	0.00100 g	0.00045 %

Graphic realization of the relative uncertainty of measurement | process accuracy

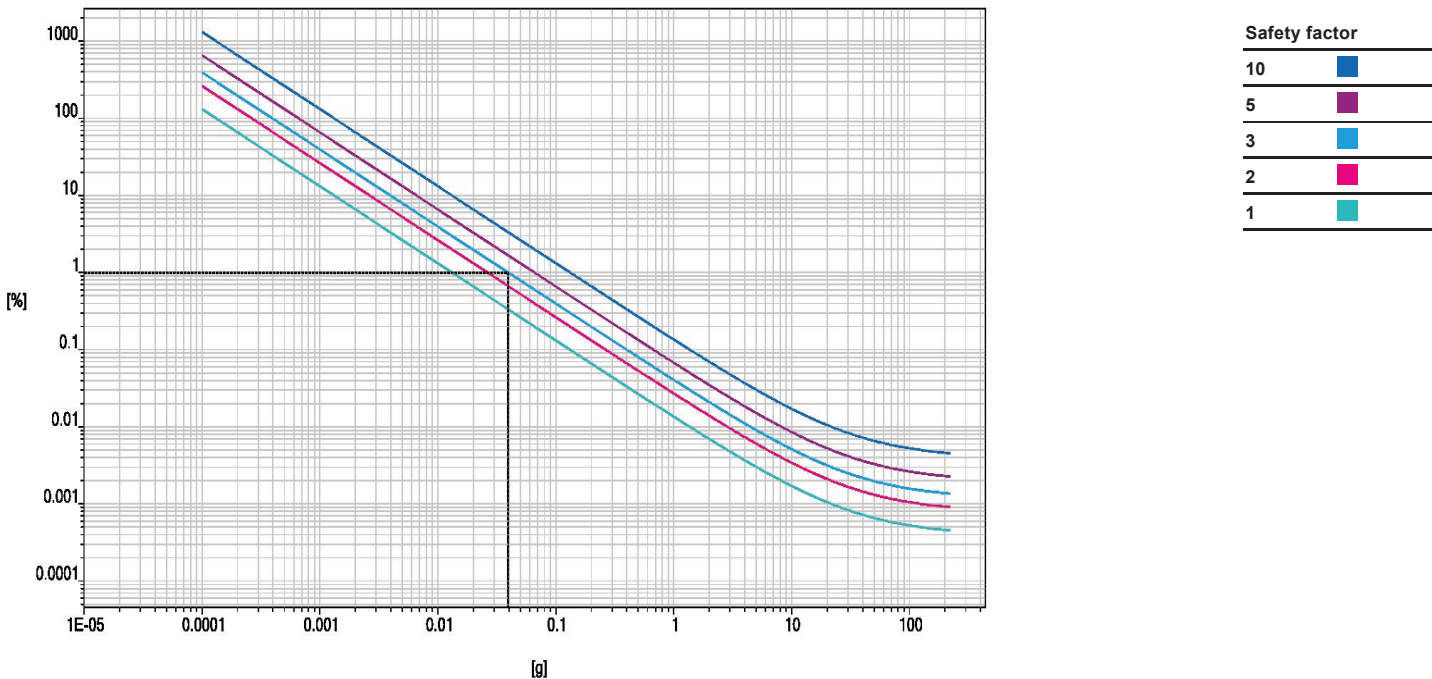

Displayed example

Process accuracy	1.00 %
Safety factor	3
Minimum sample weight	0.0395 g



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL.0-2717-3000-29 FAX.0-2719-9484



Certificate of Calibration

Cert. No.: 24TM632

Page : 1 of 3

Equipment : Hot Air Oven
Manufacturer : Memmert
Model : UFE 500
Serial No. : G511.1572
ID No. : RYG_EN0010

REVIEW BY *Thanitak.*
APPROVED BY *D. Jansen.*
NEXT CAL DATE..... 21/09/25

Submitted by : ALS Laboratory Group (Thailand) Co.,Ltd. (Rayong Branch)
616/10 Moo 5 T. Maenam Khu,
A. Pluakdaeng,
Rayong 21140 Thailand

Location : Oven Room

Received Order : 21 March 2024
Calibration Date : 21 March 2024
Ambient Temperature : (26 ± 10) °C
Relative Humidity : (50 ± 30) %

Calibrated by : Man Pattanapongpaiboon

Approved by :

Approved Signatory

() Pornthippa Tameyakul
() Unnopphol Harachai
(✓) Suwit Imjai

Issue Date : 22 March 2024

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.



Equipment : Hot Air Oven
Condition As-Received : Used Item
Reference : 2403-0563OC-1
Procedure Used :-

Cert. No.: 24TM632

Page : 2 of 3

Calibration were conducted using calibration procedure CP-OT02 according to direct measurement method with Data Acquisition which connected with Resistance Temperature Detector (RTD) and Thermocouple Type T.

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

<u>Instrument</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Traceable</u>	<u>Due Date</u>
1) Data Acquisition	MY57013711	23LM115	TPA	11 Jul 2024

2. This certificate is valid only to the item calibrated on date and place of calibration.


3. This certification is traceable to the International System of Unit.

Remark : TPA : Technology Promotion Association (Thailand - Japan)

Result of Calibration :- (*) Without Adjustment

Function of UUC* : Temperature Source

Fresh air setting : Close

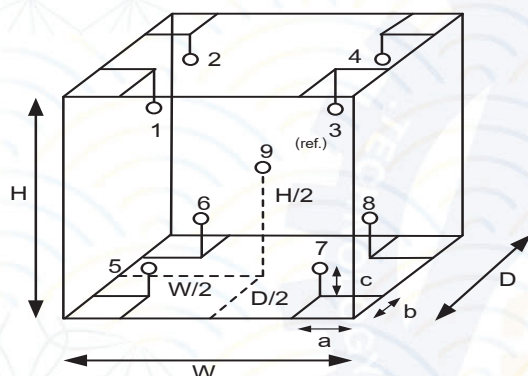

Environment during calibration		
	Beginning	Finished
Temp. (°C)	27	27
REL.Humid. (%)	57	59
AC Supply (Volt)	222	224

**Ref. Std. ID No.: @
Calibration Point**

Position :	(180) °C	(104) °C
1	18-18TC-01	18-18RTD-01
2	18-18TC-02	18-18RTD-02
3	18-18TC-03	18-18RTD-03
4	18-18TC-04	18-18RTD-04
5	18-18TC-05	18-18RTD-05
6	18-18TC-06	23-18RTD-06
7	18-18TC-07	18-18RTD-07
8	18-18TC-08	22-18RTD-08
9 (ref.)	18-18TC-09	18-18RTD-09

Probe Installation Details :

a = 5.0 cm
b = 5.0 cm
c = 5.0 cm

Dimension of Chamber :

D = 0.40 m
W = 0.56 m
H = 0.48 m
Capacity = 0.11 m³



Equipment : Hot Air Oven
Condition As-Received : Used Item
Reference : 2403-0563OC-1
Result of Calibration :- (*) Without Adjustment
Function of UUC* : Temperature Source
Fresh air setting : Close

Cert. No.: 24TM632

Page : 3 of 3

Calibration Point (°C)	UUC* Setting (°C)	UUC* Reading (°C)	Temperature stability (± °C)	Temperature uniformity (°C)	Overall Variation (°C)	Coverage Factor <i>k</i>
104.0	104.0	104.0	0.051	0.59	0.62	2
180.0	180.0	180.0	0.15	1.3	1.7	2

Calibration Point (°C)	Measured Temperature (°C)									Uncertainty (±°C)
	Position									
	1	2	3	4	5	6	7	8	9 (ref.)	
104.0	103.921	103.786	103.757	103.759	103.950	103.817	104.213	103.672	103.673	0.42
180.0	179.614	179.270	179.145	179.599	180.001	180.423	180.293	180.629	179.429	1.1

Average* : The average of 30 values in each position.

Temperature stability : One-half of the greatest maximum difference of measured temperature at any one sensor.

Temperature uniformity : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.

Overall Variation : The Difference of the maximum and minimum measured temperatures throughout observation.

UUC* : Unit Under Calibration

Note : The reported uncertainty of measurement was included stability and excluded uniformity .

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-



Metrology

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110, Thailand.

Saraburi Tel : +66 3627 3096 Fax : +66 3627 3100

Bangkok Tel : +668 9205 6851 , +669 8247 2360

Website : www.scieco.co.th E-Mail : calibrate@scg.com



Certificate No. T250454

Page 1 of 3

Certificate of Calibration

Equipment : Chamber (Oven)

Manufacturer : MEMMERT

Model : UF 110

Serial No. : B423.0853

Customer Code : RYG_EN0213

ID No. : T5884A5

Customer : ALS Laboratory Group (Thailand) Co.,Ltd. (Rayong Branch)

616/10 Moo 5 T.Maenam Khu,

A.Plukdaeng, Rayong 21140

Customer Location : ENVIRONMENT LABORATORY

Date of Receipt : 12 March 2025

Calibrated By : Sujjar Naknakred (Site Calibration Manager)

Approved By : Boonchai Boonchai Suriyawong (Site Calibration Manager)

Date of Issue : 21 MAR 2025



The uncertainties are for a confidence probability of approximately 95%.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standard laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Metrology.

Certificate No. T250454

Page 2 of 3

Calibration Report

Equipment : Chamber (Oven)
Date of Calibration : 19 March 2025
Environment : Temperature : 26.5-26.9 °C
Line Voltage : 223.9-231.3 V
Relative Humidity : 55 - 65 %RH

Condition of this results of calibration :

1. This equipment was calibrated by insert nine resistance thermometer detectors into its chamber , the other one resistance thermometer detector use for ambient temperature measurement . The calibration was done in according to WI-T20 (based on ASTM E145-94 (Reapproved 2019) and AS2853-1986) .

All data show below were final values and the initial data from customer request . The temperature scale used was based on ITS - 90 .

2. Reference Standard Instrument :

Instrument	Model	Instrument No.	Certificate No.	Due Date
RTD	100 ohm	27-(CH1-10)	T240709	19 April 2025
DATA LOGGER	34970A	T149	T240709	19 April 2025

3. This certificate is traceable to :

National Institute of Metrology (Thailand) through Metrological Center (NSC-TISI-TIS 17025 CALIBRATION 0244.)

4. Condition of calibrated item : good

Equipment Description :

Time Constant 1 Hour 44 Minute At 104 °C
Fresh Air Damper ☐ Open ☐ Min ☐ Medium ☐ Max
☒ Close
☐ Not Available

5. Adjustment :

() without adjustment


(X) after adjustment

Approved By Jon Lei

Certificate No. T250454

Page 3 of 3

Calibration Report

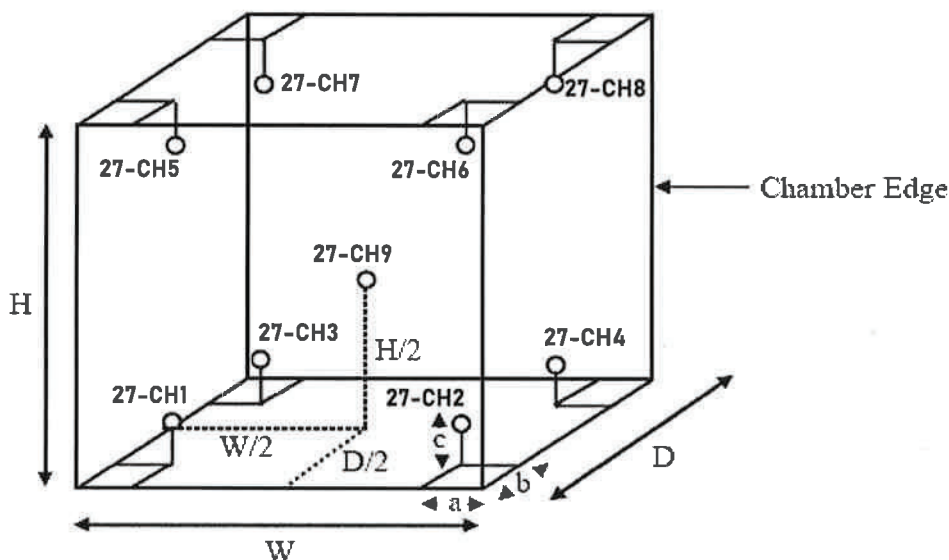

Remark : Internal Dimensions of Chamber : W (Width) = 56 cm. , H (Height) = 48 cm. and D (Depth) = 40 cm.
Size of Installed Standard sensor number 27-CH1 to number 27-CH8 : a = 5 cm. ,b = 5 cm. and c = 5 cm.
Size of Installed Standard sensor number 27-CH9 : W/2 = 56 cm./2 , H/2 = 48 cm./2 and D/2 = 40cm./2

Measurement Results

Average Standard Reading at each position (°C)									
Calibration Point	27-CH1	27-CH2	27-CH3	27-CH4	27-CH5	27-CH6	27-CH7	27-CH8	27-CH9
104	103.84	104.10	104.10	104.48	103.73	104.14	103.95	103.57	104.22
180	179.41	179.92	180.80	181.37	179.54	179.52	179.82	179.41	180.31

Chamber (Oven)			Temperature Distribution				
Setting °C	Reading (°C)		Average (°C)	Stability (± °C)	Uniformity (°C)	Uncertainty (± °C)	Coverage Factor k
	Min , Max	Average					
104.0	103.9 , 104.1	104.0	104.01	0.08	0.65	0.42	2.00
180.0	-	180.0	180.01	0.17	1.26	0.49	2.00

* The quoted uncertainty exclude "uniformity"

The calibration result apply only the above calibrated item.

The result of test was found accurate as shown on date and place of test only.

The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor k which for a t-distribution, providing a level of confidence of approximately 95 % .

End of Certificate.

Approved By. _____





TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL.0-2717-3000-29 FAX.0-2719-9484



Certificate of Calibration

Cert. No.: 24TM635

Page : 1 of 3

Equipment : Water Bath
Manufacturer : Memmert
Model : WNB22
Serial No. : L513.0648
ID No. : RYG_EN0061

Submitted by : ALS Laboratory Group (Thailand) Co.,Ltd. (Rayong Branch)
616/10 Moo 5, T. Maenam Khu,
A. Pluakdaeng,
Rayong 21140, Thailand

Location : Wet Chemistry Lab

Received Order : 21 March 2024

Calibration Date : 21 March 2024

Ambient Temperature : (26 ± 10) °C

Relative Humidity : (50 ± 30) %

Calibrated by : Man Pattanapongpaiboon

Approved by :

Approved Signatory

() Pornthippa Tameyakul

() Unnoppol Harachai

(✓) Suwit Imjai

Issue Date : 23 March 2024

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.



Equipment : Water Bath
Condition As-Received : Used Item
Reference : 2403-0563OC-4
Procedure Used :-

Cert. No.: 24TM635

Page : 2 of 3

Calibration were conducted using in-house calibration procedure CP-OT04 Based on ASTM E715 according to direct measurement method with Data Acquisition which connected with Industrial Platinum Resistance Thermometer (IPRT).

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

<u>Instrument</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Traceable</u>	<u>Due Date</u>
1) Data Acquisition	MY57013711	23LM115	TPA	11 Jul 2024

2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certification is traceable to the International System of Unit.


Remark : TPA : Technology Promotion Association (Thailand - Japan)

Result of Calibration :- (*) Without Adjustment

Function of UUC* : Temperature Source

Heat transfer medium used : Water

	<u>Environmental</u>		<u>AC Voltage Supply</u>
	(°C)	(%R.H.)	(Volt)
Beginning of Calibration	25	55	222
Finished of Calibration	25	57	223

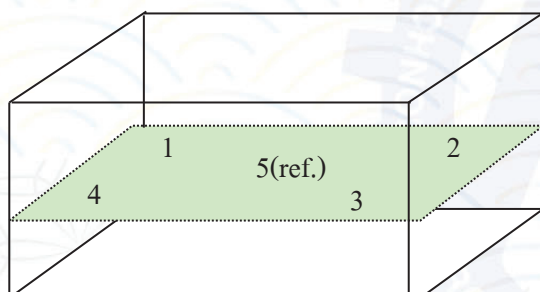

Front

<u>Position :</u>	<u>Ref. Std. ID No.:</u>
1	4803988-001
2	4803988-002
3	4803988-003
4	4803988-004
5(ref.)	4803988-005



Equipment : Water Bath
Condition As-Received : Used Item
Reference : 2403-0563OC-4
Result of Calibration :- (*) Without Adjustment
Function of UUC* : Temperature Source

Cert. No.: 24TM635

Page : 3 of 3

Calibration point (°C)	UUC* Setting (°C)	UUC* Reading (°C)	Average* Standard Reading (°C)					Uncertainty (± °C)
			Position					
			1	2	3	4	5 (ref.)	
85.0	85.0	85.0	84.428	84.424	84.489	84.507	84.477	0.18

Calibration point (°C)	Uniformity (°C)	Stability (± °C)	Coverage Factor <i>k</i>
85.0	0.19	0.11	2

Average* : The average of 30 values in each position.

Uniformity : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.


Stability : One-half of the greatest maximum difference of measured temperature at any one probe.

UUC* : Unit Under Calibration

Note : The reported uncertainty of measurement was included stability and excluded uniformity.

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-



Automation Service Co.,Ltd.

Head Office : 929,929/1 Soi Pattanakarn 30,
Pattanakarn Road, Suanluang, Bangkok
Tel: 02-319-9994 Fax: 02-319-9596
www.automation.co.th

Sales & Service Center

Rayong : 1/15 Huaypong Rd., Muang, Rayong [T. 038-692-152]
Lamphun : 122/5 M.4, Ban Klang, Muang, Lamphun [T. 053-581-876]
Prachinburi : 688 M.10, Thatum, Srimahaphote, Prachinburi [T. 037-208-880]

MTOC : L-0614/2024

Report No. : ALS-799/01

ASI Maintenance Report

Instrument : Automatic Sample Injector Measuring : Vial 40 mL
Model : ASI-L Place of Installation : -
Serial No. : H57415200799 Department : LABOLATORY
Manufacture : Shimadzu

Customer : ALS Laboratory Group (Thailand) Co.,Ltd.
104 Phatthanakan 40, Phatthanakan Rd.,
Khwaen Suan Luang, Khet Suan Luang,
Bangkok 10250 Thailand

Date of Maintenance : 26 / 06 / 2024


Ambient Condition : Temperature $25.5 \pm 5^\circ\text{C}$
: Humidifier $58 \pm 15\% \text{RH}$

REVIEW BY	Ubon S.
APPROVED BY	Siriluk P.
NEXT CAL. DATE	26/6/27

Maintenance By : T. Somri
(Mr. Tawatchai Somri)
Technician

Approved By : N. Phungsomsak
(Mr. Nipon Phungsomsak)
Technician Manager

User Name : Siriluk P.
(Mr.)



Automation Service Co.,Ltd.

Head Office : 929,929/1 Soi Pattanakarn 30,
Pattanakarn Road, Suanluang, Bangkok
Tel: 02-319-9994 Fax: 02-319-9596
www.automation.co.th

Sales & Service Center

Rayong : 1/15 Huaypong Rd., Muang, Rayong [T. 038-692-152]
Lamphun : 122/5 M.4, Ban Klang, Muang, Lamphun [T. 053-581-876]
Prachinburi : 688 M.10, Thatum, Srimahaphote, Prachinburi [T. 037-208-880]

MTOC : L-0614/2024

Report No. : ALS-799/01

Maintenance Sheet

Customer : ALS Laboratory

Date : 26 / 06 / 2024

Model : ASI-L

Serial No. H57415200799

Item	Carry out maintenance work	Result	Exchange	Comment
1.	Arm Drive section	O.K.		
	Check Arm Drive Belt for wear and tension	O.K.		
	Check grease of Screw Arm Drive	O.K.		
2.	Rinse pump (only ASI-V 24ml, 40ml)	O.K.		
	Check pump rate(>40mL/min)	O.K.		
	Check pump and tube connection for leakage	O.K.		
	Check if outlet flow is in proper condition	O.K.		
3.	Check and if necessary exchange consumable, Maintenance parts	O.K.		See appropriate list of maintenance parts
4.	Check Stirrer [When installed]	O.K.		
5.	Verify ASI function via mechanical check	O.K.		


Inspection by :

T. Somri

(Mr. Tawatchai Somri)
Technician

SHIMADZU ANALYZER

2/3



Automation Service Co.,Ltd.

Head Office : 929,929/1 Soi Pattanakarn 30,
Pattanakarn Road, Suanluang, Bangkok
Tel: 02-319-9994 Fax: 02-319-9596
www.automation.co.th

Sales & Service Center

Rayong : 1/15 Huaypong Rd., Muang, Rayong [T. 038-692-152]
Lamphun : 122/5 M.4, Ban Klang, Muang, Lamphun [T. 053-581-876]
Prachinburi : 688 M.10, Thatum, Srimahaphote, Prachinburi [T. 037-208-880]

MTOC : L-0614/2024

Report No. : ALS-799/01

List of Consumable, Maintenance parts

Pos.	Part Number	Part Name	Result	Exchange	Recommended Interval
1.	017-27021-01	Grease Paste, Lubricant 100g	O.K.	√	1 time per year
2.	032-22661-02	Belt, 60S2m596, Arm Drive	O.K.		1 time per year Depending on condition
3.	034-03067-02	Spring, F-642, Arm Drive	O.K.		Depending on condition
4.	042-00405-11	Pump Head, for ASI Rinse Pump (only ASI-V 24mL, 40mL)	O.K.		After 300 h of operating
5.	638-41448-01	Std. Needle Type1 24mL, 40mL* (for tube 2, 1x1, 6), [Sparge needle]	N/A		Depending on condition
6.	638-41448-02	Std. Needle Type1 125mL* (for tube 2, 1x1, 6)	N/A		Depending on condition
7.	631-41660-03	Flare Pipe 2x1,5x700mm* (for Standard Needle Type1 24mL,40mL, 125mL)	N/A		Depending on condition (may cut to origin length 600mm)
8.	638-41450-01	Needle for Suspended Particles,* 0,8mm (only ASI-V 24mL, 40mL)	N/A		Depending on condition
9.	638-41450-01	Std. Needle Type2 125mL* (for tube 1,4x0,9)	N/A		Depending on condition
10.	638-41472-01	Std. Needle Type2 24mL, 40mL* (for tube 1,4x0,9)	O.K.		Depending on condition
11.	631-41660-02	Flare Pipe 1,4x0,9x600mm* (for Suspended + Needle Type2)	O.K.		Depending on condition
12.	638-41449-01	Double Needle , only 24mL,40mL (simultaneous sparge type)*	N/A		Depending on condition
13.	631-41660-01	Flare Pipe 1,1x0,6x600mm* (for Double Needle 24mL,40mL)	N/A		Depending on condition


*Note: needed parts depending on installed needle types!

Inspection by :

T. Somri

(Mr. Tawatchai Somri)
Technician

SHIMADZU ANALYZER



Automation Service Co.,Ltd.

Head Office : 929,929/1 Soi Pattanakarn 30,
Pattanakarn Road, Suanluang, Bangkok
Tel: 02-319-9994 Fax: 02-319-9596
www.automation.co.th

Sales & Service Center

Rayong : 1/15 Huaypong Rd., Muang, Rayong [T. 038-692-152]
Lamphun : 122/5 M.4, Ban Klang, Muang, Lamphun [T. 053-581-876]
Prachinburi : 688 M.10, Thatum, Srimahaphote, Prachinburi [T. 037-208-880]

MTOC : L-0613/2024

Report No. : ALS-416/01

TOC-L Maintenance Report

Instrument : Total Organic Carbon Analyzer Measuring : TC 0 ~ 30000 mg/L
Model : TOC-LCSH Place of Installation : -
Serial No. : H54425300416 Department : LABORATORY
Manufacture : Shimadzu

Customer : ALS Laboratory Group (Thailand) Co.,Ltd.
104 Phatthanakan 40, Phatthanakan Rd.,
Khwaen Suan Luang, Khet Suan Luang,
Bangkok 10250 Thailand

Date of Maintenance : 26 / 06 / 2024

Ambient Condition : Temperature $25.5 \pm 5^\circ\text{C}$
: Humidifier $58 \pm 15\% \text{RH}$

REVIEW BY Ubon S.

APPROVED BY Siriluk P.

NEXT CAL. DATE 26/6/25


Maintenance By : T. Somri
(Mr. Tawatchai Somri)
Technician

Approved By : N. Phungsomsak
(Mr. Nipon Phungsomsak)
Technician Manager

User Name : Siriluk P.
()

SHIMADZU ANALYZER

1/4



Automation Service Co.,Ltd.

Head Office : 929,929/1 Soi Pattanakarn 30,
Pattanakarn Road, Suanluang, Bangkok
Tel: 02-319-9994 Fax: 02-319-9596
www.automation.co.th

Sales & Service Center

Rayong : 1/15 Huaypong Rd., Muang, Rayong [T. 038-692-152]
Lamphun : 122/5 M.4, Ban Klang, Muang, Lamphun [T. 053-581-876]
Prachinburi : 688 M.10, Thatum, Srimahaphote, Prachinburi [T. 037-208-880]

MTOC : L-0613/2024

Report No. : ALS-416/01

Maintenance Sheet

Customer : ALS Laboratory

Date : 26 / 06 / 2024

Model : TOC-LCSH


Serial No. H54425300416

Item	Carry out maintenance work	Result	Exchange	Comment
1.	Check functionality of the device			
	Check furnace temperature (Standard cat. 680 °C / for TN cat. 720 °C)	O.K.		
	Check dehumidifier temperature (1 °C)	O.K.		
	Check the entire flow line related to leakage	O.K.		
	Check baseline status (OK)	O.K.		
	Check carrier gas pressure (200 ±10 kPa)	O.K.		
	Check carrier gas flow rate (150 mL/min)	O.K.		
2.	Tubes			
	Check all tubing for contamination, if necessary clean them	O.K.		
	Check all tubing for tight connection	O.K.		
3.	Container and Drainage			
	Fill up humidifier with pure water to max. level	O.K.		
	Check filling of dilution water and acid container	O.K.		
	Rinse Drain Pot, after wards refill again with pure water	O.K.		
	Check if outlet flow is in proper conditions	O.K.		
4.	TC and IC Injection			
	Clean injector Block	O.K.		
	Check injector Block for wear	O.K.		
	Check injection tube adjustment	O.K.		
	Check injection for leakage	O.K.		
	Check injection for clogging	O.K.		
5.	IC Measurement (N-type)			
	Check acidification in syringe			
	Check sparging in syringe			
6.	Eye check of 8-Port valve, for sample residues or moist spots that indicate possible leakage	O.K.		
7.	Check and if necessary exchange consumable, Maintenance parts	O.K.		See list of consumable, maintenance parts

Inspection by :

T. Somri

(Mr. Tawatchai Somri)
Technician



Automation Service Co.,Ltd.

Head Office : 929,929/1 Soi Pattanakarn 30,
Pattanakarn Road, Suanluang, Bangkok
Tel: 02-319-9994 Fax: 02-319-9596
www.automation.co.th

Sales & Service Center

Rayong : 1/15 Huaypong Rd., Muang, Rayong [T. 038-692-152]
Lamphun : 122/5 M.4, Ban Klang, Muang, Lamphun [T. 053-581-876]
Prachinburi : 688 M.10, Thatum, Srimahaphote, Prachinburi [T. 037-208-880]

MTOC : L-0613/2024

Report No. : ALS-416/01


Item	Carry out maintenance work	Result	Exchange	Comment
8.	Due to instrument condition, clean the instrument inside and outside.	O.K.		
9.	After checking the system and exchanging of consumable and maintenance parts a new 1-3 point calibration have to be done.	O.K.		Addition test 1.
10.	After wards the calibration perform check sample measurement.	O.K.		Addition test 2.

Addition test

Test no.	Test conditions	Meas. value	Result
1.	Calibration TC standard solution at 0, 0.1, 0.5, 1, 5 10, 20 injection volume 50 µL No. of measurement 2 times (Max.3)		Attachment : ALS-416/01 Page 1/4 -2/4
	Criteria : $R^2 = 0.995$ or more	0.9996	Pass
2.	Measurement of reagent water and TC standard solution at 5.0 mg/L injection volume 50 µL No. of measurement 2 times (Max.3) and calculate accuracy by <u>Meas. of TC standard - Meas. of Reagent water</u>		Attachment : ALS-416/01 Page 3/4 - 4/4
	Criteria : Accuracy %Recovery 10% or less	5.216 - 0.2800 = 4.936 ppm	Pass

Inspection by : T. Somri

(Mr. Tawatchai Somri)
Technician



Automation Service Co.,Ltd.

Head Office : 929,929/1 Soi Pattanakarn 30,
Pattanakarn Road, Suanluang, Bangkok
Tel: 02-319-9994 Fax: 02-319-9596
www.automation.co.th

Sales & Service Center

Rayong : 1/15 Huaypong Rd., Muang, Rayong [T. 038-692-152]
Lamphun : 122/5 M.4, Ban Klang, Muang, Lamphun [T. 053-581-876]
Prachinburi : 688 M.10, Thatum, Srimahaphote, Prachinburi [T. 037-208-880]

MTOC : L-0613/2024

Report No. : ALS-416/01

List of Consumable, Maintenance parts

Pos.	Part Number	Part Name	Result	Exchange	Recommended Interval
1.	036-11209-84	O-ring, 4D P10A (Viton , for TC,IC Slider)	O.K.	√	1 time per year, Depending on condition
2.	036-11219-84	O-ring, 4D P20 (for sealing TC-Combustion tube)	O.K.	√	1 time per year, Depending on condition
3.	638-15025	O-ring, PIFE (for TC,IC-Slider)	O.K.	√	1 time per year, Depending on condition
4.	630-00105-01	Platinum net, (2pcs-set) (to support catalyst)	O.K.	√	6 month same time as catalyst exchange
5.	630-00557	Silica Wool (to support catalyst)	O.K.	√	6 month same time as catalyst exchange
6.	630-00992	Halogen Scrubber	O.K.	√	6 month
7.	630-00996	High Sensitivity TC Catalyst (When installed)	N/A		Depending on condition
8.	638-60116	Regular Catalyst (33g) (When installed)	O.K.	√	6 month
9.	638-56251-01	8-Port valve rotor	O.K.		1 time per year
10.	638-41323	TC-Combustion Tube	O.K.	√	6 month same time as catalyst exchange
11.	631-43404-01	Packing, gasket slider (for TC-Injection tube)	O.K.		1 time per year, Depending on condition
12.	638-59296	Syringe 5mL	O.K.		Depending on condition
13.	638-59296-01	Plunger Tip (for syringe 5mL)	O.K.		6 month
14.	042-00405-11	IC reagent supply pump head	O.K.		1 time per year
15.	630-00999	CO2-Absorber (for cell space purge)	O.K.		1 time per year
16.	630-00964	Molecular Sieves 13x	O.K.	√	1 time per year

Note. Table indicates the guidelines replacement periods when NPOC measurement is performed on sample that are comparatively as clean as tap water ,use standard catalyst and at a rate of about 500 sample per month (operating five days a week)

Inspector By

T. Somri

(Mr. Tawatchai Somri)
Technician

TOC-Control L Report

ALS
2024_06_26_001_PM.tlx

Instr. Information

Instrument Options
Catalyst

TOC/ASI/IC Unit/
Regular Sensitivity

Cal. Curve


Sample Name: Untitled
Sample ID: Untitled
Cal. Curve: TC 0.1 - 20 ppm.2024_06_26_13_54_50.cal
Status: Completed

Type	Anal.
Standard	TC

Conc: 0.000mg/L

No.	Area	Inj. Vol.	Aut. Dil.	Rem.	Ex.	Date / Time
1	0.7202	50uL	1.000	*****		6/26/2024 1:59:37 PM
2	0.5997	50uL	1.000	*****		6/26/2024 2:01:47 PM


Acid Add. 0.000%
Mean Area 0.6600
SD Area 0.08521
CV Area 12.91%

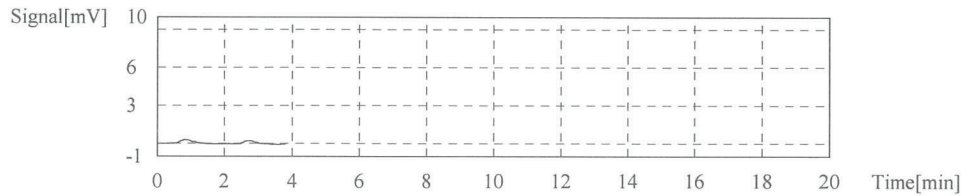

Conc: 0.1000mg/L

No.	Area	Inj. Vol.	Aut. Dil.	Rem.	Ex.	Date / Time
1	1.249	50uL	10.00	*****		6/26/2024 2:08:39 PM
2	1.139	50uL	10.00	*****		6/26/2024 2:11:28 PM


Acid Add. 0.000%
Mean Area 1.194
SD Area 0.07778
CV Area 6.51%

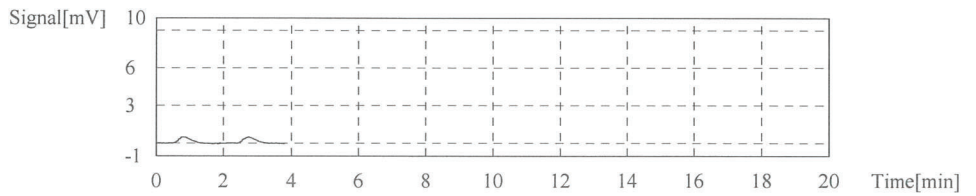

Conc: 0.5000mg/L

No.	Area	Inj. Vol.	Aut. Dil.	Rem.	Ex.	Date / Time
1	1.899	50uL	2.000	*****		6/26/2024 2:17:43 PM
2	1.779	50uL	2.000	*****		6/26/2024 2:19:52 PM

Acid Add. 0.000%
Mean Area 1.839
SD Area 0.08485
CV Area 4.61%

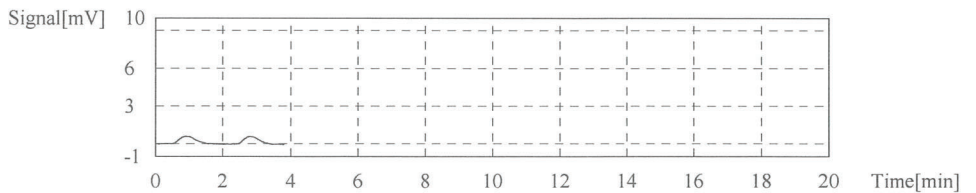


Conc: 1.000mg/L

TOC-Control L Report

ALS
2024_06_26_001_PM.tlx

No.	Area	Inj. Vol.	Aut. Dil.	Rem.	Ex.	Date / Time
1	3.121	50uL	1.000	*****	E	6/26/2024 2:22:58 PM
2	2.930	50uL	1.000	*****		6/26/2024 2:25:08 PM
3	2.899	50uL	1.000	*****		6/26/2024 2:27:18 PM


Acid Add. 0.000%
Mean Area 2.915
SD Area 0.02192
CV Area 0.75%

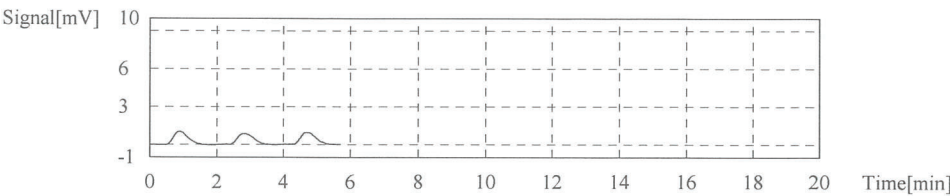

Conc: 5.000mg/L

No.	Area	Inj. Vol.	Aut. Dil.	Rem.	Ex.	Date / Time
1	12.98	50uL	4.000	*****		6/26/2024 2:34:18 PM
2	13.01	50uL	4.000	*****		6/26/2024 2:37:06 PM


Acid Add. 0.000%
Mean Area 13.00
SD Area 0.02121
CV Area 0.16%

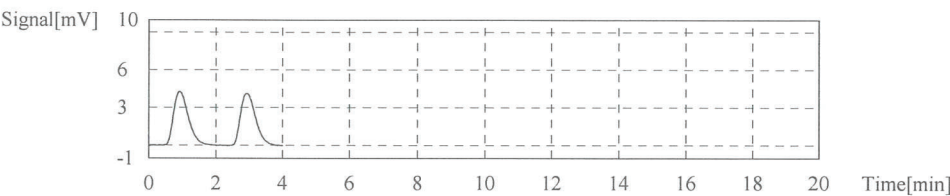

Conc: 10.00mg/L

No.	Area	Inj. Vol.	Aut. Dil.	Rem.	Ex.	Date / Time
1	25.20	50uL	2.000	*****		6/26/2024 2:43:28 PM
2	25.42	50uL	2.000	*****		6/26/2024 2:45:58 PM


Acid Add. 0.000%
Mean Area 25.31
SD Area 0.1556
CV Area 0.61%

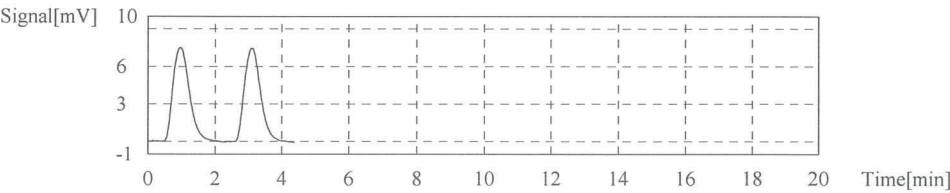


Conc: 20.00mg/L

No.	Area	Inj. Vol.	Aut. Dil.	Rem.	Ex.	Date / Time
1	48.40	50uL	1.000	*****		6/26/2024 2:49:27 PM
2	48.06	50uL	1.000	*****		6/26/2024 2:52:01 PM

Acid Add. 0.000%
Mean Area 48.23
SD Area 0.2404
CV Area 0.50%

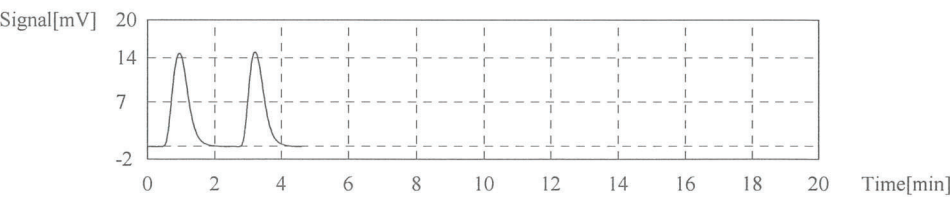

Slope: 2.388
Intercept 0.000
r^2 0.9996
r 0.9998
RSE(%) N/A
Zero Shift Yes

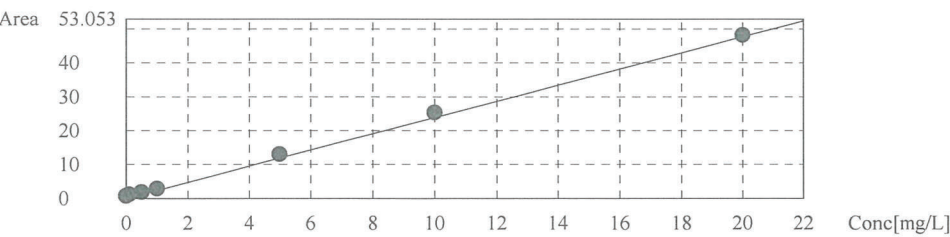

TOC-Control L Report

ALS
2024_06_26_001_PM.tlx

Instr.Information

Instrument Options
Catalyst

TOC/ASI/IC Unit/
Regular Sensitivity

Sample

Sample Name:
Sample ID:
Origin:
Status
Chk. Result

Std. TC
5 ppm
TC 0.1 - 20 ppm.cal
Completed

Type	Anal.	Manual Dilution	Result
Unknown	TC	1.000	TC:5.216mg/L


1. Det

Anal.: TC

No.	Area	Conc.	Inj. Vol.	Aut. Dil.	Ex.	Cal. Curve	Date / Time
1	12.50	5.235mg/L	50uL	1.000		TC 0.1 - 20 ppm.2024_06_26_13_54_50.cal	6/26/2024 3:01:28 PM
2	12.41	5.197mg/L	50uL	1.000		TC 0.1 - 20 ppm.2024_06_26_13_54_50.cal	6/26/2024 3:03:42 PM

Mean Area
Mean Conc.

12.46
5.216mg/L

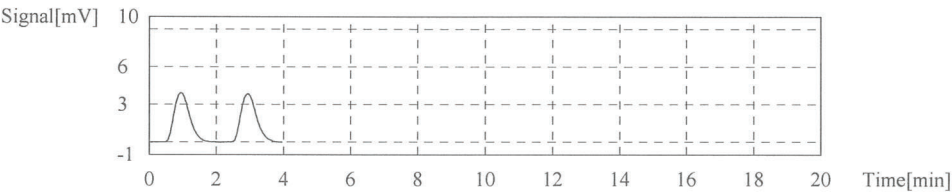

TOC-Control L Report

ALS
2024_06_26_001_PM.tlx

Instr.Information

Instrument Options
Catalyst

TOC/ASI/IC Unit/
Regular Sensitivity

Sample

Sample Name:
Sample ID:
Origin:
Status
Chk. Result

water
Untitled
TC 0.1 - 20 ppm.cal
Completed

Type	Anal.	Manual Dilution	Result
Unknown	TC	1.000	TC:0.2800mg/L


1. Det

Anal.: TC

No.	Area	Conc.	Inj. Vol.	Aut. Dil.	Ex.	Cal. Curve	Date / Time
1	0.6729	0.2818mg/L	50uL	1.000		TC 0.1 - 20 ppm.2024_06_26_13_54_50.cal	6/26/2024 3:08:11 PM
2	0.6642	0.2782mg/L	50uL	1.000		TC 0.1 - 20 ppm.2024_06_26_13_54_50.cal	6/26/2024 3:10:21 PM

Mean Area
Mean Conc.

0.6685
0.2800mg/L

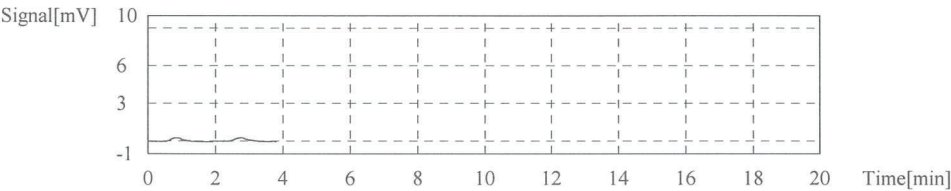

Certificate of System Qualification

GC-OQ

REVIEW BY	<i>Jinda K.</i>
APPROVED BY	<i>Tanyatorm M.</i>
NEXT CAL. DATE	<i>21 Oct 24</i>

System ID: CN11461066
Organization Name: ALS Laboratory Group (Thailand) Co., Ltd.
Organization Location: 104 Soi 40 Phatthanakan Rd, Khwang Suan Luang, Khet Suan Luang, Bangkok 10250

Date: April 21, 2023 3:26:38 PM
EQP Name: AgilentRecommended
EQP Revision: GC.02.52
Overall Qualification Status: Pass

CDS Logon Verification - GC

Logon: Saenguthai Tarak

Overall CDS Logon Verification - GC Test Status

Pass

System Inspection and Basic Safety and Operation

Name: 7890

Setpoint Status: Pass

Overall System Inspection and Basic Safety and Operation Test Status

Pass

Inlet Pressure Decay

Name: 7890

Front SSL

Setpoint Status:

Pass

Pressure: 25.0 psi

Pressure Change: -0.1 psi /5 minutes

Agilent Recommended: ≥ -2.0 and ≤ 0.5

Date: April 21, 2023 3:26:38 PM
System ID: CN11461066

Overall Inlet Pressure Decay Test Status

Pass

Inlet Pressure Accuracy

Name: 7890

Front

SSL

Setpoint Status:

Pass

Setpoint

Actual

Inlet Pressure: 25.0 psi

25.2 psi

Accuracy:

0.2 psi

Agilent Recommended:

<= 1.2

Overall Inlet Pressure Accuracy Test Status

Pass

Inlet Pressure Decay

Name: 7890

Back

SSL

Setpoint Status:

Pass

Pressure:

25.0 psi

Pressure Change:

0.0 psi /5 minutes

Agilent Recommended:

>= -2.0 and <= 0.5

Overall Inlet Pressure Decay Test Status

Pass

Inlet Pressure Accuracy

Name: 7890

Back

SSL

Setpoint Status:

Pass

	Setpoint	Actual
Inlet Pressure:	25.0 psi	24.8 psi
Accuracy:		0.2 psi
Agilent Recommended:	<=	1.2

Overall Inlet Pressure Accuracy Test Status

Pass

Detector Flow Accuracy

Name:

7890

Front

FID

Setpoint Status:

Pass

Flow Type:

Fuel

Setpoint:

30.0

mL/min

Measured Flow:

28.9

mL/min

Accuracy:

1.1

mL/min

Agilent Recommended:

<=

10.0

% setpoint

(

3.0

mL/min

)

Limit is percentage of setpoint or 0.5 ml/minute, whichever is largest.

Setpoint Status:

Pass

Flow Type:

Oxidizer

Setpoint:

400.0

mL/min

Measured Flow:

400

mL/min

Accuracy:

0.0

mL/min

Agilent Recommended:

<=

10.0

% setpoint

(

40.0

mL/min

)

Limit is percentage of setpoint or 0.5 ml/minute, whichever is largest.

Setpoint Status:

Pass

Flow Type:

Makeup

Setpoint:

25.0

mL/min

Measured Flow:

24.9

mL/min

Accuracy:

0.1

mL/min

Agilent Recommended:

<=

10.0

% setpoint

(

2.5

mL/min

)

Limit is percentage of setpoint or 0.5 ml/minute, whichever is largest.

Date:

April 21, 2023 3:26:38 PM

System ID:

CN11461066

Overall Detector Flow Accuracy Test Status

Pass

Detector Flow Accuracy

Name: 7890

Back FID

Setpoint Status: Pass

Flow Type: Fuel

Setpoint: 30.0 mL/min

Measured Flow: 30.7 mL/min

Accuracy: 0.7 mL/min

Agilent Recommended: ≤ 10.0 % setpoint (3.0 mL/min)

Limit is percentage of setpoint or 0.5 mL/minute, whichever is largest.

Setpoint Status: Pass

Flow Type: Oxidizer

Setpoint: 400.0 mL/min

Measured Flow: 399 mL/min

Accuracy: 1.0 mL/min

Agilent Recommended: ≤ 10.0 % setpoint (40.0 mL/min)

Limit is percentage of setpoint or 0.5 mL/minute, whichever is largest.

Setpoint Status: Pass

Flow Type: Makeup

Setpoint: 25.0 mL/min

Measured Flow: 24.6 mL/min

Accuracy: 0.4 mL/min

Agilent Recommended: ≤ 10.0 % setpoint (2.5 mL/min)

Limit is percentage of setpoint or 0.5 mL/minute, whichever is largest.

Overall Detector Flow Accuracy Test Status

Pass

GC Oven Temperature Accuracy

Name: 7890

Date: April 21, 2023 3:26:38 PM

System ID: CN11461066

Setpoint Status: Pass

Zone: Oven

Setpoint/Actual

Temperature: 230.0 230.6 °C

Accuracy: 0.6 °C

Agilent Recommended: ≥ -1.0 % setpoint in K (-5.0 °C) ≤ 1.0 % setpoint in K (5.0 °C)**Setpoint Status:** Pass

Zone: Oven

Setpoint/Actual

Temperature: 100.0 100.9 °C

Accuracy: 0.9 °C

Agilent Recommended: ≥ -1.0 % setpoint in K (-3.7 °C) ≤ 1.0 % setpoint in K (3.7 °C)**Overall GC Oven Temperature Accuracy Test Status**

Pass

GC Oven Temperature Stability

Name: 7890

Setpoint Status: Pass

Setpoint/Average

Temperature: 100.0 100.8833 °C

Stability: 0.1 °C

Agilent Recommended: ≤ 0.5 **Overall GC Oven Temperature Stability Test Status**

Pass

Scouting Run

Tested Combination1 Front SSL / Front FID

Injection Tower

Name: 7693A

Setpoint Status:

Completed

Injection Volume on Column:

1.0 uL

Overall Scouting Run Status

Completed

Noise and Drift

Tested Combination1

Front

SSL

/ Front

FID

Name:

7890

Setpoint Status:

Pass

Base Signal:

22.7 pA

ASTM Noise

pA

0.06

<=

0.10

Drift

pA/Hr

0.05

<=

2.50

Agilent Recommended:

Status:

Pass

Pass

Overall Noise and Drift Test Status

Pass

Injection Precision

Tested Combination1

Front

SSL

/ Front

FID

Name:

7693A

Setpoint Status:

Pass

Injection Volume on Column:

1.0 uL

Area RSD:

0.32

%

Retention Time RSD:

0.67

%

Agilent Recommended:

<=

3.00

<=

1.00

Overall Injection Precision Test Status

Pass

Signal to Noise

Date:

April 21, 2023 3:26:38 PM

System ID:

CN11461066

Tested Combination1 Front SSL / Front FID

Injection Tower

Name: 7890

Setpoint Status: Pass

Signal to Noise: 721755

Agilent Recommended: \geq 300000

Overall Signal to Noise Test Status

Pass

Scouting Run

Tested Combination2 Back SSL / Back FID

Injection Tower

Name: 7693A

Setpoint Status: Completed

Injection Volume on Column: 1.0 μ L

Overall Scouting Run Status

Completed

Noise and Drift

Tested Combination2 Back SSL / Back FID

Name: 7890

Setpoint Status: Pass

Base Signal: 22.6 pA

ASTM Noise

pA

0.07

 \leq 0.10

Agilent Recommended:

Status: Pass

Drift

pA/Hr

0.09

 \leq 2.50

Pass

Overall Noise and Drift Test Status

Pass

Injection Precision

Tested Combination2

Back

SSL

/ Back

FID

Name:

7693A

Setpoint Status:

Pass

Injection Volume on Column:

1.0

uL

Area RSD:

1.28

%

Retention Time RSD:

0.83

%

Agilent Recommended:

<=

3.00

<=

1.00

Overall Injection Precision Test Status

Pass

Signal to Noise

Tested Combination2

Back

SSL

/ Back

FID

Injection Tower

Name:

7890

Setpoint Status:

Pass

Signal to Noise:

2404398

Agilent Recommended:

>=

300000

Overall Signal to Noise Test Status

Pass

Instrument Details

Purpose

This section describes the as found system configuration.

Details

System

System ID	CN11461066
Manufacturer	Agilent Technologies
Name	7890
Flow Data Input	Manual Data
Temperature Data Input	Manual Data or Other Data Logging

Tested Combination1

Injection Technique	Injection Tower
Sampler Identifier	Sampler 2
Inlet	Front
Detector	Front
LTM Included?	No

Tested Combination2

Injection Technique	Injection Tower
Sampler Identifier	Sampler 3
Inlet	Back
Detector	Back
LTM Included?	No

Sampler 1

Manufacturer	Agilent Technologies
Type	Tray
Name	7693A
Model Number	G4514A
Serial Number	CN15380030
Firmware Revision	A.11.01
Vial Heater	Not installed

Sampler 2

Manufacturer	Agilent Technologies
Type	Injection Tower
Name	7693A
Model Number	G4513A
Serial Number	CN16280128
Firmware Revision	A.10.09
Usage	Sample Injection
Location	Front
Syringe Volume (µL)	10

Sampler 3

Manufacturer	Agilent Technologies
Type	Injection Tower
Name	7693A
Model Number	G4513A
Serial Number	CN10340103
Firmware Revision	A.10.09
Usage	Sample Injection
Location	Back
Syringe Volume (µL)	10

Mainframe 1

Manufacturer	Agilent Technologies
Name	7890
Model Number	G3440A
Serial Number	CN11461066
Firmware Revision	Version 4.27
Oven Type	Standard

Inlet 1

Manufacturer	Agilent Technologies
Name	7890
Type	SSL
Location	Front
Carrier Gas	Helium
Control Type	Electronic Pressure Control (EPC)
Purged Inlet	Yes

Inlet 2

Manufacturer	Agilent Technologies
Name	7890
Type	SSL
Location	Back
Carrier Gas	Helium
Control Type	Electronic Pressure Control (EPC)
Purged Inlet	Yes

Detector 1

Manufacturer	Agilent Technologies
Name	7890
Type	FID
Adapter	Capillary
Control Type	Electronic Pressure Control (EPC)
Location	Front
Makeup Gas	Nitrogen

Detector 2

Manufacturer	Agilent Technologies
Name	7890
Type	FID
Adapter	Capillary
Control Type	Electronic Pressure Control (EPC)
Location	Back
Makeup Gas	Nitrogen

Electronic Signature

Purpose

This signature page was created and published because the ACE sign-off action was executed, which is valid for the entire document, including attachments. The ACE sign-off is an electronic signature that requires two distinct identification components: unique username and personal password. The Agilent representative who has delivered this service understands the meaning and legal status of an electronic signature. As a trained official operator, the Agilent representative has a unique password and logon to access ACE and electronically sign this document. (Other e-signatures can be applied to this document using a Document Content Management or other suitable method defined in your data access and control procedures.)

Details

Full Name of Signer:	Saenguthai Tarak
Logged On User Name:	saenguthai.tarak@non.agilent.com
Signature Creation Date:	April 21, 2023
Reason for Signature:	Executed protocol and published this original version of document

Regulatory Disclaimer

This document provides a protocol to verify and record instrument configuration and evidence of proper operation. It has been prepared from our interpretation of applicable regulations as well as industry best practices. The document is designed to provide an important component of a complete compliance package. Validation depends upon many factors and use of this protocol alone does not assure compliance. Agilent Technologies makes no promises or representations as to its sufficiency for any specific regulatory program.

Warranty

Agilent Technologies makes no warranty of any kind to this material, including but not limited to, the implied warranties or merchantability and fitness for a particular purpose. Agilent Technologies shall not be liable for errors contained herein or for incidental or consequential damages in connection with the furnishing, performance, or use of this material.

User Name: saenguthal.tarak
 Hostname: LAPTOP-CQ3SKOMV

System Id: CN11461066
 Print Date: April 21, 2023 3:26:40 PM

GC-6_BKK_EN0127_ALS Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
April 21, 2023 11:21:36 AM	Audit	SessionCreated	Session	None
April 21, 2023 11:21:36 AM	Start	Configuration	Session	None
April 21, 2023 11:21:36 AM	Audit	Entitlement	Licensing	User is Nonpaying and does not require an unlock code
April 21, 2023 11:22:04 AM	Audit	EqpLoaded	Session	EQP details for primary technique [Gc] - File path: [ProtocolPacks/Gc/Configurations/02.52/Gc.02.52.eqp], EQP File Name: [Gc.02.52.eqp], EQP Name: [AgilentRecommended], Protocol Revision :[Gc.02.52]
April 21, 2023 11:22:06 AM	End	Configuration	Session	None
April 21, 2023 11:22:14 AM	Start	Qualification	Session	OQ
April 21, 2023 11:22:14 AM	Start	Execution	CDS Logon Verification - GC : - Qualitative test	None
April 21, 2023 11:23:14 AM	End	Execution	CDS Logon Verification - GC : - Qualitative test	Run Count : 1
April 21, 2023 11:23:16 AM	Start	Execution	System Inspection and Basic Safety and Operation - 7890: - Qualitative Test - No setpoints associated	None
April 21, 2023 11:23:35 AM	End	Execution	System Inspection and Basic Safety and Operation - 7890: - Qualitative Test - No setpoints associated	Run Count : 1
April 21, 2023 11:23:37 AM	Start	Execution	Inlet Pressure Decay - Front SSL: - Pressure Controlled Inlet - S: 25.0 psi - L: >= -2.0 psi and <= 0.5 psi	None

User Name: saenguthai.tarak
 Hostname: LAPTOP-CQ3SKOMV

System Id: CN11461066
 Print Date: April 21, 2023 3:26:40 PM

GC-6_BKK_EN0127_ALS Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
April 21, 2023 11:24:01 AM	End	Execution	Inlet Pressure Decay - Front SSL: - Pressure Controlled Inlet - S: 25.0 psi - L: >= -2.0 psi and ≤ 0.5 psi	Run Count : 1
April 21, 2023 11:24:04 AM	Start	Execution	Inlet Pressure Accuracy - Front SSL: - Pressure Controlled Inlet - S: 25.0 psi - L: ≤ 1.2 psi	None
April 21, 2023 11:24:09 AM	End	Execution	Inlet Pressure Accuracy - Front SSL: - Pressure Controlled Inlet - S: 25.0 psi - L: ≤ 1.2 psi	Run Count : 1
April 21, 2023 11:24:11 AM	Start	Execution	Inlet Pressure Decay - Back SSL: - Pressure Controlled Inlet - S: 25.0 psi - L: >= -2.0 psi and ≤ 0.5 psi	None
April 21, 2023 11:24:43 AM	End	Execution	Inlet Pressure Decay - Back SSL: - Pressure Controlled Inlet - S: 25.0 psi - L: >= -2.0 psi and ≤ 0.5 psi	Run Count : 1
April 21, 2023 11:24:45 AM	Start	Execution	Inlet Pressure Accuracy - Back SSL: - Pressure Controlled Inlet - S: 25.0 psi - L: ≤ 1.2 psi	None
April 21, 2023 11:24:51 AM	End	Execution	Inlet Pressure Accuracy - Back SSL: - Pressure Controlled Inlet - S: 25.0 psi - L: ≤ 1.2 psi	Run Count : 1
April 21, 2023 11:24:53 AM	Start	Execution	Detector Flow Accuracy - Front FID: - Type : Fuel - S: 30.0 mL/min - L: ≤ 10.0% setpoint	None
April 21, 2023 11:25:20 AM	Audit	Data	Detector Flow Accuracy - Front FID: - Type : Fuel - S: 30.0 mL/min - L: ≤ 10.0% setpoint	Manual Data Entry
April 21, 2023 11:25:25 AM	End	Execution	Detector Flow Accuracy - Front FID: - Type : Fuel - S: 30.0 mL/min - L: ≤ 10.0% setpoint	Run Count : 1

User Name: saenguthai.tarak
 Hostname: LAPTOP-CQ3SKOMV

System Id: CN11461066
 Print Date: April 21, 2023 3:26:40 PM

GC-6_BKK_EN0127_ALS Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
April 21, 2023 11:25:26 AM	Start	Execution	Detector Flow Accuracy - Front FID: - Type : Oxidizer - S: 400.0 mL/min - L: <= 10.0% setpoint	None
April 21, 2023 11:25:40 AM	Audit	Data	Detector Flow Accuracy - Front FID: - Type : Oxidizer - S: 400.0 mL/min - L: <= 10.0% setpoint	Manual Data Entry
April 21, 2023 11:25:42 AM	End	Execution	Detector Flow Accuracy - Front FID: - Type : Oxidizer - S: 400.0 mL/min - L: <= 10.0% setpoint	Run Count : 1
April 21, 2023 11:25:44 AM	Start	Execution	Detector Flow Accuracy - Front FID: - Type : Makeup - S: 25.0 mL/min - L: <= 10.0% setpoint	None
April 21, 2023 11:26:01 AM	Audit	Data	Detector Flow Accuracy - Front FID: - Type : Makeup - S: 25.0 mL/min - L: <= 10.0% setpoint	Manual Data Entry
April 21, 2023 11:26:04 AM	End	Execution	Detector Flow Accuracy - Front FID: - Type : Makeup - S: 25.0 mL/min - L: <= 10.0% setpoint	Run Count : 1
April 21, 2023 11:26:05 AM	Start	Execution	Detector Flow Accuracy - Back FID: - Type : Fuel - S: 30.0 mL/min - L: <= 10.0% setpoint	None
April 21, 2023 11:26:19 AM	Audit	Data	Detector Flow Accuracy - Back FID: - Type : Fuel - S: 30.0 mL/min - L: <= 10.0% setpoint	Manual Data Entry
April 21, 2023 11:26:22 AM	End	Execution	Detector Flow Accuracy - Back FID: - Type : Fuel - S: 30.0 mL/min - L: <= 10.0% setpoint	Run Count : 1
April 21, 2023 11:26:24 AM	Start	Execution	Detector Flow Accuracy - Back FID: - Type : Oxidizer - S: 400.0 mL/min - L: <= 10.0% setpoint	None
April 21, 2023 11:26:38 AM	Audit	Data	Detector Flow Accuracy - Back FID: - Type : Oxidizer - S: 400.0 mL/min - L: <= 10.0% setpoint	Manual Data Entry

Page 3 / 11

Date: April 21, 2023 3:26:38 PM
 System ID: CN11461066

User Name: saenguthai.tarak
 Hostname: LAPTOP-CQ3SKOMV

System Id: CN11461066
 Print Date: April 21, 2023 3:26:40 PM

GC-6_BKK_EN0127_ALS Transaction log:

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
April 21, 2023 11:26:43 AM	End	Execution	Detector Flow Accuracy - Back FID: - Type : Oxidizer - S: 400.0 mL/min - L: <= 10.0% setpoint	Run Count : 1
April 21, 2023 11:26:45 AM	Start	Execution	Detector Flow Accuracy - Back FID: - Type : Makeup - S: 25.0 mL/min - L: <= 10.0% setpoint	None
April 21, 2023 11:27:01 AM	Audit	Data	Detector Flow Accuracy - Back FID: - Type : Makeup - S: 25.0 mL/min - L: <= 10.0% setpoint	Manual Data Entry
April 21, 2023 11:27:05 AM	End	Execution	Detector Flow Accuracy - Back FID: - Type : Makeup - S: 25.0 mL/min - L: <= 10.0% setpoint	Run Count : 1
April 21, 2023 11:27:07 AM	Start	Execution	GC Oven Temperature Accuracy - 7890: - Temperature : Oven - S: 230.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	None
April 21, 2023 11:27:33 AM	Audit	Data	GC Oven Temperature Accuracy - 7890: - Temperature : Oven - S: 230.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	Manual Data Entry
April 21, 2023 11:27:35 AM	End	Execution	GC Oven Temperature Accuracy - 7890: - Temperature : Oven - S: 230.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	Run Count : 1
April 21, 2023 11:27:37 AM	Start	Execution	GC Oven Temperature Accuracy - 7890: - Temperature : Oven - S: 100.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	None
April 21, 2023 11:27:54 AM	Audit	Data	GC Oven Temperature Accuracy - 7890: - Temperature : Oven - S: 100.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	Manual Data Entry

User Name: saenguthai.tarak
 Hostname: LAPTOP-CQ3SKOMV

System Id: CN11461066
 Print Date: April 21, 2023 3:26:40 PM

GC-6_BKK_EN0127_ALS Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
April 21, 2023 11:27:57 AM	End	Execution	GC Oven Temperature Accuracy - 7890: - Temperature : Oven - S: 100.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	Run Count : 1
April 21, 2023 11:27:59 AM	Start	Execution	GC Oven Temperature Stability - 7890: - Temperature : Oven - S: 100.0°C - L: <= 0.5°C	None
April 21, 2023 11:29:07 AM	Audit	Data	GC Oven Temperature Stability - 7890: - Temperature : Oven - S: 100.0°C - L: <= 0.5°C	Manual Data Entry
April 21, 2023 11:29:10 AM	End	Execution	GC Oven Temperature Stability - 7890: - Temperature : Oven - S: 100.0°C - L: <= 0.5°C	Run Count : 1
April 21, 2023 11:29:12 AM	Start	Execution	GC Scouting Run - Injection Tower, Front SSL, Front FID: - Part of System Preparation - No limits associated	None
April 21, 2023 11:30:27 AM	Audit	Data	GC Scouting Run - Injection Tower, Front SSL, Front FID: - Part of System Preparation - No limits associated	Data files Path : C:\Users\Public\Documents\C hemStation\3\Data\OQ_GC-6 _ALS_2023-04-20\OQ_GC-6 _2023 2023-04-20 14-36-08\F_SC01.D\FID1A.c h
April 21, 2023 11:31:04 AM	End	Execution	GC Scouting Run - Injection Tower, Front SSL, Front FID: - Part of System Preparation - No limits associated	Run Count : 1
April 21, 2023 11:31:07 AM	Start	Execution	Noise and Drift - Front FID: - Detector FID - L (Noise): <= 0.10 pA - L (Drift): <= 2.50 pA/hour	None

User Name: saenguthai.tarak
 Hostname: LAPTOP-CQ3SKOMV

System Id: CN11461066
 Print Date: April 21, 2023 3:26:40 PM

GC-6_BKK_EN0127_ALS Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
April 21, 2023 11:31:43 AM	Audit	Data	Noise and Drift - Front FID: - Detector FID - L (Noise): <= 0.10 pA - L (Drift): <= 2.50 pA/hour	Data files Path : C:\Users\Public\Documents\C hemStation\3\Data\OQ_GC-6 _ALS_2023-04-20\OQ_GC-6 _2023 2023-04-20 14-36-08\ND-01-005F.D\FID 1A.ch
April 21, 2023 11:32:00 AM	End	Execution	Noise and Drift - Front FID: - Detector FID - L (Noise): <= 0.10 pA - L (Drift): <= 2.50 pA/hour	Run Count : 1
April 21, 2023 11:32:03 AM	Start	Execution	Injection Precision - Injection Tower, Front SSL, Front FID: - GC - L (Area): <= 3.00% - L (Ret. Time): <= 1.00%	None
April 21, 2023 11:32:23 AM	Start	Execution	Injection Precision - Injection Tower, Front SSL, Front FID: - GC - L (Area): <= 3.00% - L (Ret. Time): <= 1.00%	None
April 21, 2023 11:33:55 AM	Audit	Data	Injection Precision - Injection Tower, Front SSL, Front FID: - GC - L (Area): <= 3.00% - L (Ret. Time): <= 1.00%	Data files Path : C:\Users\Public\Documents\C hemStation\3\Data\OQ_GC-6 _ALS_2023-04-20\OQ_GC-6 _2023 2023-04-20 14-36-08\Pre01-013F.D\FID 1A.ch
April 21, 2023 11:33:55 AM	Audit	Data	Injection Precision - Injection Tower, Front SSL, Front FID: - GC - L (Area): <= 3.00% - L (Ret. Time): <= 1.00%	Data files Path : C:\Users\Public\Documents\C hemStation\3\Data\OQ_GC-6 _ALS_2023-04-20\OQ_GC-6 _2023 2023-04-20 14-36-08\Pre01-014F.D\FID 1A.ch

User Name: saenguthal.tarak
 Hostname: LAPTOP-CQ3SKOMV

System Id: CN11461066
 Print Date: April 21, 2023 3:26:40 PM

GC-6_BKK_EN0127_ALS Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
April 21, 2023 11:33:55 AM	Audit	Data	Injection Precision - Injection Tower, Front SSL, Front FID: - GC - L (Area): <= 3.00% - L (Ret. Time): <= 1.00%	Data files Path : C:\Users\Public\Documents\C hemStation\3\Data\OQ_GC-6 _ALS_2023-04-20\OQ_GC-6 _2023 2023-04-20 14-36-08\Pre01-015F.D\FID 1A.ch
April 21, 2023 11:33:55 AM	Audit	Data	Injection Precision - Injection Tower, Front SSL, Front FID: - GC - L (Area): <= 3.00% - L (Ret. Time): <= 1.00%	Data files Path : C:\Users\Public\Documents\C hemStation\3\Data\OQ_GC-6 _ALS_2023-04-20\OQ_GC-6 _2023 2023-04-20 14-36-08\Pre01-016F.D\FID 1A.ch
April 21, 2023 11:33:59 AM	Audit	Data	Injection Precision - Injection Tower, Front SSL, Front FID: - GC - L (Area): <= 3.00% - L (Ret. Time): <= 1.00%	Data files Path : C:\Users\Public\Documents\C hemStation\3\Data\OQ_GC-6 _ALS_2023-04-20\OQ_GC-6 _2023 2023-04-20 14-36-08\Pre01-017F.D\FID 1A.ch
April 21, 2023 11:33:59 AM	Audit	Data	Injection Precision - Injection Tower, Front SSL, Front FID: - GC - L (Area): <= 3.00% - L (Ret. Time): <= 1.00%	Data files Path : C:\Users\Public\Documents\C hemStation\3\Data\OQ_GC-6 _ALS_2023-04-20\OQ_GC-6 _2023 2023-04-20 14-36-08\Pre01-018F.D\FID 1A.ch
April 21, 2023 11:35:00 AM	End	Execution	Injection Precision - Injection Tower, Front SSL, Front FID: - GC - L (Area): <= 3.00% - L (Ret. Time): <= 1.00%	Run Count : 1
April 21, 2023 11:35:04 AM	Start	Execution	Signal to Noise - Injection Tower, Front SSL, Front FID: - Detector FID - L: >= 300000	None

User Name: saenguthai.tarak
 Hostname: LAPTOP-CQ3SKOMV

System Id: CN11461066
 Print Date: April 21, 2023 3:26:40 PM

GC-6_BKK_EN0127_ALS Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
April 21, 2023 11:35:28 AM	Audit	Data	Signal to Noise - Injection Tower, Front SSL, Front FID: - Detector FID - L: >= 300000	Data files Path : C:\Users\Public\Documents\C hemStation\3\Data\OQ_GC-6 _ALS_2023-04-20\OQ_GC-6 _2023 2023-04-20 14-36-08\SN_Front.D\FID1A. ch
April 21, 2023 11:36:00 AM	End	Execution	Signal to Noise - Injection Tower, Front SSL, Front FID: - Detector FID - L: >= 300000	Run Count : 1
April 21, 2023 11:36:03 AM	Start	Execution	GC Scouting Run - Injection Tower, Back SSL, Back FID: - Part of System Preparation - No limits associated	None
April 21, 2023 11:36:36 AM	Audit	Data	GC Scouting Run - Injection Tower, Back SSL, Back FID: - Part of System Preparation - No limits associated	Data files Path : C:\Users\Public\Documents\C hemStation\3\Data\OQ_GC-6 _ALS_2023-04-20\OQ_GC-6 _2023 2023-04-20 14-36-08\B_SC01.D\FID2B.c h
April 21, 2023 11:37:30 AM	End	Execution	GC Scouting Run - Injection Tower, Back SSL, Back FID: - Part of System Preparation - No limits associated	Run Count : 1
April 21, 2023 11:37:32 AM	Start	Execution	Noise and Drift - Back FID: - Detector FID - L (Noise): <= 0.10 pA - L (Drift): <= 2.50 pA/hour	None

User Name: saenguthal.tarak
 Hostname: LAPTOP-CQ3SKOMV

System Id: CN11461066
 Print Date: April 21, 2023 3:26:40 PM

GC-6_BKK_EN0127_ALS Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
April 21, 2023 11:38:06 AM	Audit	Data	Noise and Drift - Back FID: - Detector FID - L (Noise): <= 0.10 pA - L (Drift): <= 2.50 pA/hour	Data files Path : C:\Users\Public\Documents\C hemStation\3\Data\OQ_GC-6 _ALS_2023-04-20\OQ_GC-6 _2023 2023-04-20 14-36-08\ND-01-005B.D\FID 2B.ch
April 21, 2023 11:38:23 AM	End	Execution	Noise and Drift - Back FID: - Detector FID - L (Noise): <= 0.10 pA - L (Drift): <= 2.50 pA/hour	Run Count : 1
April 21, 2023 11:38:32 AM	Start	Execution	Injection Precision - Injection Tower, Back SSL, Back FID: - GC - L (Area): <= 3.00% - L (Ret. Time): <= 1.00%	None
April 21, 2023 11:38:51 AM	Start	Execution	Injection Precision - Injection Tower, Back SSL, Back FID: - GC - L (Area): <= 3.00% - L (Ret. Time): <= 1.00%	None
April 21, 2023 11:40:17 AM	Audit	Data	Injection Precision - Injection Tower, Back SSL, Back FID: - GC - L (Area): <= 3.00% - L (Ret. Time): <= 1.00%	Data files Path : C:\Users\Public\Documents\C hemStation\3\Data\OQ_GC-6 _ALS_2023-04-20\OQ_GC-6 _2023_Pre 2023-04-21 10-37-32\Pre11-004B.D\FID 2B.ch
April 21, 2023 11:40:17 AM	Audit	Data	Injection Precision - Injection Tower, Back SSL, Back FID: - GC - L (Area): <= 3.00% - L (Ret. Time): <= 1.00%	Data files Path : C:\Users\Public\Documents\C hemStation\3\Data\OQ_GC-6 _ALS_2023-04-20\OQ_GC-6 _2023_Pre 2023-04-21 10-37-32\Pre11-005B.D\FID 2B.ch

User Name: saenguthai.tarak
 Hostname: LAPTOP-CQ3SKOMV

System Id: CN11461066
 Print Date: April 21, 2023 3:26:40 PM

GC-6_BKK_EN0127_ALS Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
April 21, 2023 11:40:17 AM	Audit	Data	Injection Precision - Injection Tower, Back SSL, Back FID: - GC - L (Area): <= 3.00% - L (Ret. Time): <= 1.00%	Data files Path : C:\Users\Public\Documents\C hemStation\3\Data\OQ_GC-6 _ALS_2023-04-20\OQ_GC-6 _2023_Pre 2023-04-21 10-37-32\Pre11-006B.D\FID 2B.ch
April 21, 2023 11:40:17 AM	Audit	Data	Injection Precision - Injection Tower, Back SSL, Back FID: - GC - L (Area): <= 3.00% - L (Ret. Time): <= 1.00%	Data files Path : C:\Users\Public\Documents\C hemStation\3\Data\OQ_GC-6 _ALS_2023-04-20\OQ_GC-6 _2023_Pre 2023-04-21 10-37-32\Pre11-007B.D\FID 2B.ch
April 21, 2023 11:40:21 AM	Audit	Data	Injection Precision - Injection Tower, Back SSL, Back FID: - GC - L (Area): <= 3.00% - L (Ret. Time): <= 1.00%	Data files Path : C:\Users\Public\Documents\C hemStation\3\Data\OQ_GC-6 _ALS_2023-04-20\OQ_GC-6 _2023_Pre 2023-04-21 10-37-32\Pre11-008B.D\FID 2B.ch
April 21, 2023 11:40:21 AM	Audit	Data	Injection Precision - Injection Tower, Back SSL, Back FID: - GC - L (Area): <= 3.00% - L (Ret. Time): <= 1.00%	Data files Path : C:\Users\Public\Documents\C hemStation\3\Data\OQ_GC-6 _ALS_2023-04-20\OQ_GC-6 _2023_Pre 2023-04-21 10-37-32\Pre11-009B.D\FID 2B.ch
April 21, 2023 11:41:29 AM	End	Execution	Injection Precision - Injection Tower, Back SSL, Back FID: - GC - L (Area): <= 3.00% - L (Ret. Time): <= 1.00%	Run Count : 1
April 21, 2023 11:41:33 AM	Start	Execution	Signal to Noise - Injection Tower, Back SSL, Back FID: - Detector FID - L: >= 300000	None

User Name: saenguthal.tarak
 Hostname: LAPTOP-CQ3SKOMV

System Id: CN11461066
 Print Date: April 21, 2023 3:26:40 PM

GC-6_BKK_EN0127_ALS Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
April 21, 2023 11:42:22 AM	Audit	Data	Signal to Noise - Injection Tower, Back SSL, Back FID: - Detector FID - L: >= 300000	Data files Path : C:\Users\Public\Documents\C hemStation\3\Data\OQ_GC-6 _ALS_2023-04-20\OQ_GC-6 _2023 2023-04-20 14-36-08\SN_Back.D\FID2B. ch
April 21, 2023 11:42:50 AM	End	Execution	Signal to Noise - Injection Tower, Back SSL, Back FID: - Detector FID - L: >= 300000	Run Count : 1
April 21, 2023 11:42:53 AM	End	Qualification	Session	OQ
April 21, 2023 11:42:53 AM	Start	Reporting	Session	None
April 21, 2023 12:01:47 PM	Audit	AceClosed	Session	None
April 21, 2023 3:16:07 PM	Audit	AceRestarted	Session	None
April 21, 2023 3:16:10 PM	Audit	SessionReloaded	Session	None
April 21, 2023 3:16:31 PM	Start	Qualification	Session	OQ
April 21, 2023 3:20:59 PM	Audit	AceRestarted	Session	None
April 21, 2023 3:21:00 PM	Audit	SessionReloaded	Session	None
April 21, 2023 3:21:07 PM	Start	Qualification	Session	OQ
April 21, 2023 3:25:45 PM	Audit	Reporting	Session	Report Generated : Certificate

C

C

ภาคผนวก จ

สำเนาหนังสือรับรองห้องปฏิบัติการวิเคราะห์เอกชน



ที่ อก ๐๓๑๐(๑)/ ๑๖๑๖๘

กรมโรงงานอุตสาหกรรม
ถนนพระรามที่ ๖ แขวงทุ่งพญาไท
เขตราชเทวี กรุงเทพฯ ๑๐๕๐๐

๒๐ พฤศจิกายน ๒๕๖๖

เรื่อง ต่ออายุหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน

เรียน กรรมการผู้จัดการ บริษัท เอแอลเอส แลบบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด

อ้างถึง คำขอขึ้นทะเบียน/ต่ออายุ/เปลี่ยนแปลงบุคลากร และชนิดสารมลพิษของห้องปฏิบัติการวิเคราะห์เอกชน
ลงวันที่ ๔ สิงหาคม ๒๕๖๖

- สิ่งที่ส่งมาด้วย ๑. รายชื่อผู้ควบคุมดูแลห้องปฏิบัติการวิเคราะห์ จำนวน ๑ แผ่น
๒. รายชื่อเจ้าหน้าที่ประจำห้องปฏิบัติการวิเคราะห์ จำนวน ๕ แผ่น
๓. ขอบข่ายสารมลพิษที่ได้รับขึ้นทะเบียนจากกรมโรงงานอุตสาหกรรม จำนวน ๓๑ แผ่น

ตามหนังสือที่อ้างถึง บริษัท เอแอลเอส แลบบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด ขอต่ออายุหนังสือ
รับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน เลขทะเบียน ว-๒๐๔ สถานที่ตั้งเลขที่ ๑๐๔ ซอยพัฒนาการ ๔๐
ถนนพัฒนาการ แขวงพัฒนาการ เขตสวนหลวง กรุงเทพมหานคร ต่อกรมโรงงานอุตสาหกรรม นั้น

กรมโรงงานอุตสาหกรรมพิจารณาแล้ว ให้บริษัท เอแอลเอส แลบบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด
ต่ออายุหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน โดยมีองค์ประกอบดังนี้

- ก. ผู้ควบคุมดูแลห้องปฏิบัติการวิเคราะห์ จำนวน ๖ ราย ตามสิ่งที่ส่งมาด้วย ๑
ข. เจ้าหน้าที่ประจำห้องปฏิบัติการวิเคราะห์ ๑๘๑ ราย ตามสิ่งที่ส่งมาด้วย ๒
ค. ขอบข่ายสารมลพิษที่ได้รับขึ้นทะเบียนให้วิเคราะห์ในน้ำเสีย น้ำใต้ดิน อากาศเสีย สิ่งปฏิกูล
หรือวัสดุที่ไม่ใช่แล้ว และดิน ตามสิ่งที่ส่งมาด้วย ๓

หนังสือฉบับนี้จะหมดอายุในวันที่ ๒ กันยายน ๒๕๖๙ หากประสงค์จะต่ออายุหนังสือ
รับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน ให้ยื่นคำขอต่ออายุพร้อมเอกสารประกอบคำขอต่อ
กรมโรงงานอุตสาหกรรม ภายใน ๓๐ วัน ก่อนวันสิ้นอายุของหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน
ทั้งนี้ สามารถยื่นคำขอผ่านระบบอิเล็กทรอนิกส์ได้ที่หน้าเว็บไซต์กรมโรงงานอุตสาหกรรม

จึงเรียนมาเพื่อทราบ

ขอแสดงความนับถือ

(นายศิริระ จันทรเจ็ด)

นักวิทยาศาสตร์เชี่ยวชาญ วิชาการแผน
ผู้อำนวยการกองวิจัยและเตือนภัยมลพิษโรงงาน
ปฏิบัติราชการแทนอธิบดีกรมโรงงานอุตสาหกรรม

กองวิจัยและเตือนภัยมลพิษโรงงาน

กลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษและทะเบียนห้องปฏิบัติการ

โทร. ๐ ๒๔๓๐ ๖๓๑๒ ต่อ ๒๑๐๓-๕

โทรสาร ๐ ๒๔๓๐ ๖๓๑๒ ต่อ ๒๑๙๙

ไปรษณีย์อิเล็กทรอนิกส์ saraban@diw.mail.go.th



“อุตสาหกรรมก้าวไกล ประเทศไทยก้าวหน้า ร่วมกันพัฒนา อุตสาหกรรมสีเขียว”



สิ่งที่ส่งมาด้วย ๑

เอกสารแนบท้ายหนังสือรับต่ออายุขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน
บริษัท เอแอลเอส แลบบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด เลขทะเบียน ว-๒๐๔
ที่ อก ๐๓๑๐(๑)/ ๑ ๖ ๑ ๖ ๘ ลงวันที่ ๒๐ พฤศจิกายน ๒๕๖๖

ก. ผู้ควบคุมดูแลห้องปฏิบัติการวิเคราะห์ จำนวน ๖ ราย

- | | |
|---------------------------------|----------------------------|
| ๑) นางสาวยุพพร จันทร์เปล่ง | ทะเบียนเลขที่ ว-๒๐๔-ค-๐๐๐๑ |
| ๒) นางสาวชัชณีย์ โกมารกุล ณ นคร | ทะเบียนเลขที่ ว-๒๐๔-ค-๐๐๐๒ |
| ๓) นายศรายุทธ จิตรานนท์ | ทะเบียนเลขที่ ว-๒๐๔-ค-๐๐๐๓ |
| ๔) นางสาวกนกกร เอนก | ทะเบียนเลขที่ ว-๒๐๔-ค-๐๐๐๔ |
| ๕) นายสุริยา สอนแก้ว | ทะเบียนเลขที่ ว-๒๐๔-ค-๐๐๐๕ |
| ๖) นายวิชาญ ชูณหรัตน์ | ทะเบียนเลขที่ ว-๒๐๔-ค-๐๐๐๖ |

รวม

เอกสารแนบท้ายหนังสือรับต่ออายุขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน

บริษัท เอแอลเอส แลบบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด

เลขทะเบียน ว-๒๐๔

ที่ อก ๐๓๑๐(๑)/ ๑๖๑๖๘

ลงวันที่ ๒๐ พฤศจิกายน ๒๕๖๖

ข. เจ้าหน้าที่ประจำห้องปฏิบัติการวิเคราะห์ จำนวน ๑๘๑ ราย

๑) นายกาจบัณฑิต กิตติศุภวณิชย์	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๐๑
๒) นายภัทรพล สว่างใจธรรม์	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๐๒
๓) นายณรรธิป เทือกชัยคำ	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๐๓
๔) นายศิริโชค พงษ์ประสม	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๐๔
๕) นายณัฐวุฒิ ด่วงแพง	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๐๕
๖) นางสาวจินดา ไชจุลธรรม	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๐๖
๗) นางสาวสาวิตรี น้อยเสงี่ยม	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๐๗
๘) นางสาวชนัญญาญจน์ อิ่มชม	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๐๘
๙) นางสาวนรินทร์ สายเส็ง	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๐๙
๑๐) นางสาวนันทวดี สมบูรณ์	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๑๐
๑๑) นางสาวศรัณยา เฉลิมธำรงค์	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๑๑
๑๒) นางสาวธัญญธร มงคลจิรวุฒิ	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๑๒
๑๓) นางสาวศิริลักษณ์ บุนนาค	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๑๓
๑๔) นายณพนธ์ จันทะพันธุ์	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๑๔
๑๕) นายนรเศรษฐ์ โกมลาลย์	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๑๕
๑๖) นายธันวา จริยา	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๑๖
๑๗) นางสาวเกศรินทร์ แก้วมัน	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๑๗
๑๘) นางสาวสุวิมล ชัยเรืองวุฒิ	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๑๘
๑๙) นางสาวสุชาดา ธรรมถาวร	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๑๙
๒๐) นางสาวเปมิกา ชัยเดชธนกุล	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๒๐
๒๑) นางสาวศศิธร หมูสวัสดิ์	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๒๑
๒๒) นางสาวเสาวลักษณ์ ภู่นาอำพร	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๒๒
๒๓) นายอภิสิทธิ์ สิงหา	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๒๓
๒๔) นายศักดิ์สิทธิ์ ไพศาลพิสุทธิ	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๒๔
๒๕) ว่าที่ร้อยตรีหญิง พรรณิภา ขำเจริญ	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๒๕
๒๖) นางจิตดา คำภูแก้ว	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๒๖
๒๗) นางสาวอรรรณ รักยง	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๒๗
๒๘) นางสาวนพรัตน์ แยมกรานต์	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๒๘
๒๙) นายจุลเดช วารินทร์	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๒๙
๓๐) นางสาวดาญรัตน์ ร้องคำ	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๓๐
๓๑) นายพรมมี ศรีปัดเนตร	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๓๑
๓๒) นายอุทิศ อุ่นลิ้ม	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๓๒
๓๓) ว่าที่ร้อยตรี เฉลิมเกียรติ อมรศรีเสริม	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๓๓
๓๔) นางสาววริยา สร้างนา	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๓๔
๓๕) นายอนุพงศ์ รัตนศรีประเสริฐ	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๓๕

วิมล

๓๖) นางสาวจุฑารัตน์...

๓๖) นางสาวจุฑารัตน์ โอนสันเทียะ
๓๗) นางสาวจารุวรรณ พิมพ์ภักฤติยา
๓๘) นางสาวปรามค์ทิพย์ กิจไพศาลศักดิ์
๓๙) นางสาวเตือนใจ ทางกลาง
๔๐) นางสาวจิราพร ศิริเวช
๔๑) นายวรกร ผุ่กรักษ์
๔๒) นายทง วิริยะสทกิจ
๔๓) นายธนิศ เจนจบ
๔๔) นายคณิศร ข้าเพชร
๔๕) นายภูวิช พรหมสะอาด
๔๖) นายธนเดช โภคาพิพัฒน์
๔๗) นายชวฤทธิ์ วงษ์จันทร์
๔๘) นายอาทิตย์ ศรีเสน
๔๙) นายเจษดินทร์ คงศักดิ์ไทย
๕๐) นายจรัส บุญยั้ง
๕๑) นายธนาณัติ เอนก
๕๒) นายอภิวัฒน์ ทุมหนู
๕๓) นางสาวสุภาขวัญ มาก
๕๔) นางสาวทัตพร ขวาลสมบูรณ์
๕๕) นางสาวธิดิมา บุญเพ็ง
๕๖) นางสาวภาณุมาศ นามวัฒน์
๕๗) นางสาวอุไรรัตน์ ทังสร้างแป้น
๕๘) นายธีรวัฒน์ ปวงสุข
๕๙) นายอิทธิพล ยะโส
๖๐) นายประพจน์ วรรณชูชัย
๖๑) นายชยธร พวงทิพย์
๖๒) นางสาวกนกวรรณ จันทบาล
๖๓) นายสิทธิโชค ธงเงิน
๖๔) นางศิวารรณ ใจบุญ
๖๕) นางสาวพรรณธิดา พุ่มคง
๖๖) นายนวกัทร ศรีวิริยะ
๖๗) นายสุวิชา ทองอ่อน
๖๘) นายวิญญู บุญตะนัย
๖๙) นายสมบูรณ์ บุตรจันทร์
๗๐) นายวิรัตน์ ไชยนะรา
๗๑) นายณฤเบศน์ เพิ่มพูน
๗๒) นายจิรณัฐ ขาวละออ
๗๓) นายอัสรี นามบุรี
๗๔) นายอัครเศรฐ จ่อสาว

ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๓๖
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๓๗
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๓๘
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๓๙
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๔๐
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๔๑
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๔๒
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๔๓
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๔๔
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๔๕
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๔๖
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๔๗
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๔๘
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๔๙
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๕๐
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๕๑
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๕๒
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๕๓
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๕๔
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๕๕
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๕๖
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๕๗
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๕๘
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๕๙
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๖๐
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๖๑
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๖๒
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๖๓
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๖๔
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๖๕
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๖๖
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๖๗
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๖๘
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๖๙
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๗๐
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๗๑
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๗๒
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๗๓
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๗๔

31/๗

๗๕) นายประเสริฐ...

๗๕) นายประเสริฐ สุระขันธ
๗๖) นายบุญกุล จันทน์นิยม
๗๗) นายพิรพงษ์ ทองคุณปรีดา
๗๘) นายณฤพล ทองนุช
๗๙) นายอนุวัฒน์ ม่วงแพ
๘๐) นายเจตศราวุฒิ บัตตะมะ
๘๑) นายกฤษณะ สายวรรณ
๘๒) นายพิชัย บุญยงค์
๘๓) นายภาณุพงศ์ โอเมวงศ์
๘๔) นายสามารถ คัมปลี
๘๕) นายสัญญาชัย โกศรีนาม
๘๖) นายณัฐวุฒิ ศรีประเสริฐ
๘๗) นายชวลิตชัย นาคพนม
๘๘) นายพงศธร ชัยทิพย์
๘๙) นายสิทธิโชค ทาสีดา
๙๐) นายธนากร อินสุตา
๙๑) นางสาววรรณิษา ขาติวันชัย
๙๒) นางสาวพิมพ์ตะวัน มินากุล
๙๓) นางสาวเพชรรัตน์ สิงห์สมบุญ
๙๔) นางสาวชญานิน พรหมจันทร์
๙๕) นายกীরติ ทวีราช
๙๖) นายจักริน หมั่นวิชา
๙๗) นายฉัตรชัย สุขเปี้ย
๙๘) นายณรรณท์ ต๊ะทองคำ
๙๙) นายดุสิตพล สอนอก
๑๐๐) นายทักษ์ดนัย อุบลศรี
๑๐๑) นายธนศร นามะภูณณา
๑๐๒) นายธิตพิงค์ บัวแดง
๑๐๓) นายณนทชัย อุปถัมภ์
๑๐๔) นายณัฐพล คุณสุทธิ
๑๐๕) นายณันท์วัฒน์ สาริน
๑๐๖) นายปิยะนัฐ พลมะศรี
๑๐๗) นายพงศ์สิริ โสมเขียว
๑๐๘) นายพีรพัฒน์ กำคำ
๑๐๙) นายภาณุพงศ์ มานิตย์
๑๑๐) นายมงคล ผลาทิพย์
๑๑๑) นายสิรินนท์ ทองอ้น
๑๑๒) นายอนเนชา ทนสมัย
๑๑๓) นายอดิศักดิ์ ผมไผ

ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๗๕
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๗๖
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๗๗
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๗๘
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๗๙
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๘๐
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๘๑
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๘๒
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๘๓
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๘๔
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๘๕
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๘๖
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๘๗
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๘๘
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๘๙
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๙๐
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๙๑
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๙๒
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๙๓
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๙๔
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๙๕
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๙๖
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๙๗
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๙๘
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๙๙
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๐๐
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๐๑
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๐๒
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๐๓
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๐๔
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๐๕
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๐๖
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๐๗
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๐๘
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๐๙
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๑๐
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๑๑
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๑๒
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๑๓

วิมล

๑๑๔) นายอนันตชัย...

๑๑๔) นายอนันตชัย วิสม
๑๑๕) นายวรวิธ คีนิก
๑๑๖) นายแสงตะวัน นະตะสັต
๑๑๗) นายยุทธพงศ์ รัตนะ
๑๑๘) นายชัยณัฐมิ ไชยชนะนิจ
๑๑๙) นายวิศรุต ศรีธรรมมา
๑๒๐) นายนนทกร เผือกผ่อง
๑๒๑) นายกำชัย สุทธะ
๑๒๒) นางสาวณัฐภรณ์ บุญตะนัย
๑๒๓) นางสาวพัชรินทร์ แสนสร้อย
๑๒๔) นายไพโรจน์ เปี่ยมพิมาย
๑๒๕) นางสาวศุภมาศ ทองมาก
๑๒๖) นางสาวลลิตา จิตรสว่าง
๑๒๗) นางสาวขไมพร เล็กภูเขียว
๑๒๘) นางสาวกฤติมาพร คำมีแก่น
๑๒๙) นางสาวสกุลรัตน์ ภาควุฒิ
๑๓๐) นางสาวไพรินทร์ ศรีรูป
๑๓๑) นางสาวทิพนันทร ผุยปัญญา
๑๓๒) นางสาวสาธิตา ปานทอง
๑๓๓) นางสาวอริสา ทองนวล
๑๓๔) นางสาวอรยา คำคล้อง
๑๓๕) นางสาวชุตติภรณ์ สุนทรสนาน
๑๓๖) นางสาวอัญชลี คำจันทร์
๑๓๗) นายบุญฤทธิ์ เอี่ยมเทศ
๑๓๘) นางสาวศุภรดา ปันมยุรา
๑๓๙) นางสาวพาณดี คุณน่าน
๑๔๐) นางสาวจิราเจต พองดา
๑๔๑) นางสาวอารยา มีชัย
๑๔๒) นางสาววิชุดา นาคผจญ
๑๔๓) นางสาวนันทิยา จันทะลุน
๑๔๔) นายกิตติพงศ์ แซ่ลี
๑๔๕) นายอนุวัติ ภูถวิล
๑๔๖) นายธีรพล แสงทอง
๑๔๗) นายศักดิ์พิพัฒน์ บุญมัน
๑๔๘) นายฐิติวัตรค์ เอมอุไร
๑๔๙) นายชัยณรงค์ ศรีบุรินทร์
๑๕๐) นางสาวอัจฉราวรรณ สอนสนอง
๑๕๑) นางสาวณัฐราพร สิงหา
๑๕๒) นายกัมเรศ แหยมโต

ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๑๔
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๑๕
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๑๖
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๑๗
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๑๘
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๑๙
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๒๐
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๒๑
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๒๒
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๒๓
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๒๔
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๒๕
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๒๖
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๒๗
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๒๘
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๒๙
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๓๐
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๓๑
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๓๒
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๓๓
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๓๔
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๓๕
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๓๖
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๓๗
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๓๘
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๓๙
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๔๐
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๔๑
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๔๒
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๔๓
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๔๔
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๔๕
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๔๖
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๔๗
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๔๘
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๔๙
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๕๐
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๕๑
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๕๒

31/10/2561

๑๕๓) นางสาวอุบล...

๑๕๓) นางสาวอุบล เคิกศิริ
๑๕๔) นางสาวมโนรัตน์ ทองบุตร
๑๕๕) นายภาคภูมิ แทนไทย
๑๕๖) นางสาวสุภาณัฐ เมล์พ่วง
๑๕๗) นางสาวพรทิศา สาตาชนม์
๑๕๘) นายเอกวิทย์ วันทะนา
๑๕๙) นายไตรมณฑล ทิพย์วรรณ
๑๖๐) นายจิรเมธ ประเสริฐสิริพงศ์
๑๖๑) นายจิรายุส เกษมสุข
๑๖๒) นายจรัสศักดิ์ ศรีวิชัย
๑๖๓) นายณัฐฤกษ์ สพานแก้ว
๑๖๔) นายบุรณศักดิ์ ปะที
๑๖๕) นายปณณวิชัย เสมอทรัพย์
๑๖๖) นายพิษณุพงษ์ ไชยา
๑๖๗) นายภัทรพงษ์ มณฑาทอง
๑๖๘) นายวสันต์ ตรีนกุล
๑๖๙) นายภาณุเดช เพชรอุด
๑๗๐) นายอนุกุล วิละแสง
๑๗๑) นายภัทรพงษ์ มีสุข
๑๗๒) นางสาวนุชวี ลีละทีป
๑๗๓) นางสาวสุภาวดี โกศรีนาม
๑๗๔) นางสาวอรณิศา เทียนคำ
๑๗๕) นางสาวพรเพ็ญ ขอบสอน
๑๗๖) นางสาววันวิสา ขอนพิกุล
๑๗๗) นางสาวอรรพรรณ เถาว์ทอง
๑๗๘) นางสาวอัยย์ลีน เมอร์วินณ์
๑๗๙) นางสาววิสรา ค่อยครอง
๑๘๐) นายวุฒิกร ศิริวรรณ
๑๘๑) นางสาวจรรววรรณ กระจ่างพันธุ์

ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๕๓
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๕๔
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๕๕
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๕๖
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๕๗
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๕๘
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๕๙
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๖๐
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๖๑
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๖๒
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๖๓
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๖๔
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๖๕
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๖๖
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๖๗
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๖๘
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๖๙
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๗๐
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๗๑
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๗๒
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๗๓
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๗๔
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๗๕
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๗๖
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๗๗
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๗๘
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๗๙
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๘๐
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๘๑

วิภา

เอกสารแนบท้ายหนังสือรับต่ออายุขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน

บริษัท เอแอลเอส แลบบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด เลขทะเบียน ว-๒๐๔

ที่ อก ๐๓๑๐(๑)/ ๑๖๑๖๘ ลงวันที่ ๒๐ พฤศจิกายน ๒๕๖๖

ค. ขอบข่ายสารมลพิษที่ได้รับขึ้นทะเบียนจากกรมโรงงานอุตสาหกรรม จำนวน ๓๗๔ รายการ

น้ำเสีย จำนวน 60 รายการ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
1	Aldicarb	High-Performance Liquid Chromatographic Method ^[4]
2	Aldicarb Sulfone	High-Performance Liquid Chromatographic Method ^[4]
3	Aldicarb Sulfoxide	High-Performance Liquid Chromatographic Method ^[4]
4	Aldrin	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
5	Arsenic	1) Digestion, Inductively Coupled Plasma Method ^[4] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method ^[4]
6	Barium	1) Digestion, Inductively Coupled Plasma Method ^[4] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method ^[4]
7	α-BHC	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
8	β-BHC	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
9	δ-BHC	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
10	γ-BHC	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
11	Biochemical Oxygen Demand	1) 5-Day BOD Test, Azide Modification Method ^[4] 2) 5-Day BOD Test, Membrane Electrode Method ^[4]
12	Carbaryl	High-Performance Liquid Chromatographic Method ^[4]
13	Carbofuran	High-Performance Liquid Chromatographic Method ^[4]
14	Cadmium	1) Digestion, Inductively Coupled Plasma Method ^[4] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method ^[4]
15	Chemical Oxygen Demand	1) Closed Reflux, Colorimetric Method ^[4] 2) Closed Reflux, Titrimetric Method ^[4]
16	Chlordane	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
17	Chromium	1) Digestion, Inductively Coupled Plasma Method ^[4] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method ^[4]
18	Color	ADMI Weighted-Ordinate Spectrophotometric Method ^[4]

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
19	Copper	1) Digestion, Inductively Coupled Plasma Method ^[4] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method ^[4]
20	Cyanide	Distillation, Colorimetric Method ^[4]
21	2,4'-DDD	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
22	4,4'-DDD	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
23	2,4'-DDE	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
24	4,4'-DDE	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
25	2,4'-DDT	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
26	4,4'-DDT	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
27	Dieldrin	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
28	Endosulfan Sulfate	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
29	Endosulfan I	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
30	Endosulfan II	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
31	Endrin	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
32	Endrin Aldehyde	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
33	Formaldehyde	Distillation, Colorimetric Method ^[3]
34	Free Chlorine	1) DPD Ferrous Titrimetric Method ^[4] 2) DPD Colorimetric Method ^[4]
35	Heptachlor	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
36	Heptachlor Epoxide	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
37	Hexavalent Chromium	Colorimetric Method ^[4]
38	3-Hydroxycarbofuran	High-Performance Liquid Chromatographic Method ^[4]
39	Lead	1) Digestion, Inductively Coupled Plasma Method ^[4] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method ^[4]

สมิ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
40	Manganese	1) Digestion, Inductively Coupled Plasma Method ^[4] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method ^[4]
41	Mercury	1) Digestion, Cold-Vapor Atomic Absorption Spectrometric Method ^[4] 2) Digestion, Inductively Coupled Plasma/ Mass spectrometric Method ^[4]
42	Methiocarb	High-Performance Liquid Chromatographic Method ^[4]
43	Methoxychlor	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
44	Methomyl	High-Performance Liquid Chromatographic Method ^[4]
45	Nickel	1) Digestion, Inductively Coupled Plasma Method ^[4] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method ^[4]
46	Oil & Grease	1) Liquid-Liquid, Partition-Gravimetric Method ^[4] 2) Soxhlet Extraction Method ^[4]
47	Oxamyl	High-Performance Liquid Chromatographic Method ^[4]
48	Propoxur	High-Performance Liquid Chromatographic Method ^[4]
49	pH	Electrometric Method ^[4]
50	Phenols	1) Distillation, Chloroform Extraction Method ^[4] 2) Distillation, Direct Photometric Method ^[4]
51	Selenium	1) Digestion, Inductively Coupled Plasma Method ^[4] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method ^[4]
52	Sulfide	Iodometric Method ^[4]
53	Temperature	Laboratory and Field Methods ^[4]
54	Total Dissolved Solids	Dried at 180 °C ^[4]
55	Total Kjeldahl Nitrogen	Semi-Micro Kjeldahl Method ^[4]
56	Total Phosphorous	Digestion, Colorimetric Method ^[4]
57	Total Suspended Solids	Dried from 103-105 °C ^[4]
58	Toxaphene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
59	Trivalent Chromium	1) Digestion, Inductively Coupled Plasma Method; Colorimetric Method; Calculation ^[4] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method; Colorimetric Method; Calculation ^[4]
60	Zinc	1) Digestion, Inductively Coupled Plasma Method ^[4] 2) Digestion, Inductively Coupled Plasma/Mass Spectrometric Method ^[4]

วิมล

น้ำใต้ดิน จำนวน 126 รายการ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
1	Acenaphthene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
2	Acetone	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[4]
3	Aldrin	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
4	Anthracene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
5	Antimony	1) Digestion, Inductively Coupled Plasma Method ^[4] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method ^[4]
6	Arsenic	1) Digestion, Inductively Coupled Plasma Method ^[4] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method ^[4]
7	Atrazine	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
8	Barium	1) Digestion, Inductively Coupled Plasma Method ^[4] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method ^[4]
9	Benz(a)anthracene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
10	Benzene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[4]
11	Benzo(b)fluoranthene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
12	Benzo(k)fluoranthene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
13	Benzoic Acid	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
14	Benzo(a)pyrene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
15	Benzo[g,h,i]perylene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
16	Beryllium	1) Digestion, Inductively Coupled Plasma Method ^[4] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method ^[4]
17	Bis(2-chloroethyl)ether	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
18	Bis(2-ethylhexyl)phthalate	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
19	Bromodichloromethane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[4]
20	Bromoform	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[4]
21	Butanol	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[4]
22	Butyl benzyl phthalate	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
23	Cadmium	1) Digestion, Inductively Coupled Plasma Method ^[4] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method ^[4]
24	Carbazole	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
25	Carbon disulfide	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[4]
26	Carbon tetrachloride	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[4]
27	Chlordane	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
28	p-Chloroaniline	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
29	Chlorobenzene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[4]
30	Chlorodibromomethane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[4]
31	Chloroform	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[4]
32	2-Chlorophenol	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
33	Chromium	1) Digestion, Inductively Coupled Plasma Method ^[4] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method ^[4]
34	Chromium (III)	1) Digestion, Inductively Coupled Plasma Method; Colorimetric Method; Calculation ^[4] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method; Colorimetric Method; Calculation ^[4]
35	Chromium (VI)	Colorimetric Method ^[4]

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
36	Chrysene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
37	Cyanide	Distillation, Colorimetric Method ^[4]
38	2,4-D	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
39	DDD	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
40	DDE	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
41	DDT	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
42	Dibenz(a,h)anthracene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
43	Di-n-Butyl Phthalate	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
44	1,2-Dichlorobenzene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[4]
45	1,3-Dichlorobenzene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[4]
46	1,4-Dichlorobenzene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[4]
47	3,3-Dichlorobenzidine	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
48	1,1-Dichloroethane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[4]
49	1,2-Dichloroethane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[4]
50	1,1-Dichloroethylene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[4]
51	cis-1,2-Dichloroethylene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[4]
52	trans-1,2-Dichloroethylene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[4]
53	2,4-Dichlorophenol	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
54	1,2-Dichloropropane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[4]
55	1,3-Dichloropropane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[4]

3m

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
56	1,3-Dichloropropene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[4]
57	Dieldrin	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
58	Diethyl Phthalate	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
59	2,4-Dimethylphenol	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
60	2,4-Dinitrophenol	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
61	2,4-Dinitrotoluene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
62	2,6-Dinitrotoluene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
63	Di-n-octyl phthalate	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
64	Endosulfan	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
65	Endrin	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
66	Ethylbenzene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[4]
67	Fluoranthene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
68	Fluorene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
69	Heptachlor	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
70	Heptachlor epoxide	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
71	Hexachlorobenzene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
72	Hexachloro-1,3-butadiene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[4]
73	n-Hexane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[4]
74	α -HCH	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
75	β -HCH	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]

3m2

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
76	γ -HCH	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
77	Hexachlorocyclopentadiene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
78	Hexachloroethane	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
79	Indeno(1,2,3-cd)pyrene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
80	Isophorone	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
81	Lead	1) Digestion, Inductively Coupled Plasma Method ^[4] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method ^[4]
82	Manganese	1) Digestion, Inductively Coupled Plasma Method ^[4] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method ^[4]
83	Mercury	1) Digestion, Cold Vapor Atomic Absorption Spectrometric Method ^[4] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method ^[4]
84	Methanol	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[4]
85	Methoxychlor	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
86	Methyl bromide	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[4]
87	Methylene chloride	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[4]
88	2-Methylphenol	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
89	2-Methylnaphthalene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
90	Methyl tert-butyl Ether	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[4]
91	Naphthalene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
92	Nickel	1) Digestion, Inductively Coupled Plasma Method ^[4] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method ^[4]
93	Nitrobenzene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
94	N-Nitrosodiphenylamine	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
95	N-Nitrosodi-n-Propylamine	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
96	Polychlorinated Biphenyls - PCB 1016 - PCB 1221 - PCB 1232 - PCB 1242 - PCB 1248 - PCB 1254 - PCB 1260	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
97	Pentachlorophenol	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
98	pH	Electrometric Method ^[4]
99	Phenanthrene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
100	Phenol	1) Distillation, Chloroform Extraction Method ^[4] 2) Distillation, Direct Photometric Method ^[4] 3) Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
101	Pyrene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
102	Selenium	1) Digestion, Inductively Coupled Plasma Method ^[4] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method ^[4]
103	Silver	1) Digestion, Inductively Coupled Plasma Method ^[4] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method ^[4]
104	Styrene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[4]
105	1,1,2,2-Tetrachloroethane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[4]
106	Tetrachloroethylene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[4]
107	Toluene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[4]
108	Toxaphene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
109	TPH (C ₅ -C ₈)	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[14,25]

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
110	TPH (C ₈ -C ₁₆)	Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method ^[9,22]
111	TPH (C ₁₆ -C ₃₅)	Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method ^[9,22]
112	1,2,4-Trichlorobenzene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[4]
113	1,1,1-Trichloroethane	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[4]
114	1,1,2-Trichloroethane	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[4]
115	Trichloroethylene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[4]
116	2,4,5-Trichlorophenol	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
117	2,4,6-Trichlorophenol	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
118	1,3,5-Trimethylbenzene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[4]
119	Vanadium	1) Digestion, Inductively Coupled Plasma Method ^[4] 2) Digestion, Inductively Coupled Plasma/Mass Spectrometric Method ^[4]
120	Vinyl acetate	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[4]
121	Vinyl chloride	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[4]
122	m-Xylene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[4]
123	o-Xylene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[4]
124	p-Xylene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[4]
125	Xylene (Total)	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[4]
126	Zinc	1) Digestion, Inductively Coupled Plasma Method ^[4] 2) Digestion, Inductively Coupled Plasma/Mass Spectrometric Method ^[4]

อากาศเสีย (ปล่อยระบาย) จำนวน 28 รายการ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
1	Antimony	1) Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method ^[5]
2	Arsenic	2) Isokinetic Sampling, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method ^[5]
3	Beryllium	1) Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method ^[5]
4	Cadmium	2) Isokinetic Sampling, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method ^[5]
5	Carbon Monoxide	1) Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method ^[5]
6	Chlorine	2) Isokinetic Sampling, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method ^[5]
7	Chromium	1) Instrumental Analyzer Method ^[5]
8	Cobalt	2) Sampling Bag Non-Dispersive Infrared Method ^[5]
9	Copper	1) Absorption Sampling, Ion Chromatographic Method ^[5]
10	Cresol	2) Isokinetic Sampling, Ion Chromatographic Method ^[5]
11	Dioxins	1) Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method ^[5]
12	Hydrogen Chloride	2) Isokinetic Sampling, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method ^[5]
13	Hydrogen Fluoride	1) Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method ^[5]
14	Hydrogen Sulfide	2) Isokinetic Sampling, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method ^[5]

3mm

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
27	Vanadium	1) Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method ^[5] 2) Isokinetic Sampling, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method ^[5]
28	Xylene	Adsorption Sampling, Gas Chromatographic Method ^[5]

สิ่งปฏิกูลหรือวัสดุที่ไม่ใช้แล้ว จำนวน 35 รายการ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
1	Aldrin	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[1,9,26] 2) Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method ^[10,26] 3) Automated Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method ^[11,26]
2	Antimony	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[1,6,16] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method ^[1,6,17] 3) Digestion, Inductively Coupled Plasma Method ^[7,16] 4) Digestion, Inductively Coupled Plasma/Mass Spectrometric Method ^[7,17]
3	Arsenic	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[1,6,16] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method ^[1,6,17] 3) Digestion, Inductively Coupled Plasma Method ^[7,16] 4) Digestion, Inductively Coupled Plasma/Mass Spectrometric Method ^[7,17]
4	Barium	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[1,6,16] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method ^[1,6,17] 3) Digestion, Inductively Coupled Plasma Method ^[7,16] 4) Digestion, Inductively Coupled Plasma/Mass Spectrometric Method ^[7,17]

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
5	Beryllium	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[1,6,16] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method ^[1,6,17] 3) Digestion, Inductively Coupled Plasma Method ^[7,16] 4) Digestion, Inductively Coupled Plasma/Mass Spectrometric Method ^[7,17]
6	Cadmium	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[1,6,16] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method ^[1,6,17] 3) Digestion, Inductively Coupled Plasma Method ^[7,16] 4) Digestion, Inductively Coupled Plasma/Mass Spectrometric Method ^[7,17]
7	Chlordane	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[1,9,26] 2) Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method ^[10,26] 3) Automated Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method ^[11,26]
8	Chromium	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[1,6,16] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method ^[1,6,17] 3) Digestion, Inductively Coupled Plasma Method ^[7,16] 4) Digestion, Inductively Coupled Plasma/Mass Spectrometric Method ^[7,17]
9	Chromium (III)	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method; Waste Extraction, Colorimetric Method; Calculation Method ^[1,6,16,19] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method; Waste Extraction, Colorimetric Method; Calculation Method ^[1,6,17,19] 3) Digestion, Inductively Coupled Plasma Method; Alkaline Digestion, Colorimetric Method; Calculation Method ^[7,8,16,19] 4) Digestion, Inductively Coupled Plasma/Mass Spectrometric Method; Alkaline Digestion, Colorimetric Method; Calculation Method ^[7,8, 17,19]

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
10	Chromium (VI)	1) Waste Extraction, Colorimetric Method ^[1,6,19]
11	Cobalt	2) Alkaline Digestion, Colorimetric Method ^[8,19] 1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[1,6,16] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method ^[1,6,17] 3) Digestion, Inductively Coupled Plasma Method ^[7,16] 4) Digestion, Inductively Coupled Plasma/Mass Spectrometric Method ^[7,17]
12	Copper	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[1,6,16] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method ^[1,6,17] 3) Digestion, Inductively Coupled Plasma Method ^[7,16] 4) Digestion, Inductively Coupled Plasma/Mass Spectrometric Method ^[7,17]
13	2,4-D	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[1,9,26] 2) Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method ^[10,26] 3) Automated Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method ^[11,26]
14	DDD	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[1,9,26] 2) Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method ^[10,26] 3) Automated Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method ^[11,26]
15	DDE	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[1,9,26] 2) Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method ^[10,26] 3) Automated Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method ^[11,26]
16	DDT	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[1,9,26]

2ml

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
17	Dieldrin	2) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[10,26] 3) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[11,26] 1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[1,9,26]
18	Endrin	2) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[10,26] 3) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[11,26] 1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[1,9,26]
19	Heptachlor	2) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[10,26] 3) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[11,26] 1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[1,9,26]
20	Lead	2) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[10,26] 3) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[11,26] 1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[1,6,16] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method ^[1,6,17] 3) Digestion, Inductively Coupled Plasma Method ^[7,16] 4) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method ^[7,17]
21	Lindane	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[1,9,26] 2) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[10,26] 3) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[11,26]

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
22	Mercury	1) Waste Extraction, Digestion, Cold-Vapor Atomic Absorption Spectrometric Method ^[1,6,20] 2) Waste Extraction, Digestion, Cold-Vapor Atomic Fluorescence Spectrometric Method ^[1,6,30] 3) Digestion, Cold-Vapor Atomic Absorption Spectrometric Method ^[20] 4) Digestion, Cold-Vapor Atomic Fluorescence Spectrometric Method ^[30] 5) Thermal Decomposition Amalgamation and Atomic Absorption Spectrometric Method ^[21]
23	Methoxychlor	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[1,9,26] 2) Soxhlet Extraction, Gas Chromatographic / Mass Spectrometric Method ^[10,26] 3) Automated Soxhlet Extraction, Gas Chromatographic / Mass Spectrometric Method ^[11,26]
24	Mirex	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[1,9,26] 2) Soxhlet Extraction, Gas Chromatographic / Mass Spectrometric Method ^[10,26] 3) Automated Soxhlet Extraction, Gas Chromatographic / Mass Spectrometric Method ^[11,26]
25	Molybdenum	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[1,6,16] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method ^[1,6,17] 3) Digestion, Inductively Coupled Plasma Method ^[7,16] 4) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method ^[7,17]
26	Nickel	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[1,6,16] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method ^[1,6,17] 3) Digestion, Inductively Coupled Plasma Method ^[7,16] 4) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method ^[7,17]
27	Polychlorinated biphenyls (PCBs) - Aroclor 1016 - Aroclor 1221 - Aroclor 1232 - Aroclor 1242 - Aroclor 1248 - Aroclor 1254 - Aroclor 1260	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[1,9,26] 2) Soxhlet Extraction, Gas Chromatographic Method ^[10,26] 3) Automated Soxhlet Extraction, Gas Chromatographic Method ^[11,26]

31m

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
28	<ul style="list-style-type: none"> - 2-Chlorobiphenyl - 2,3-Dichlorobiphenyl - 2,2',5-Trichlorobiphenyl - 2,4',5-Trichlorobiphenyl - 2,2',3,5'-Tetrachlorobiphenyl - 2,2',5,5'-Tetrachlorobiphenyl - 2,3',4,4'-Tetrachlorobiphenyl - 2,2',3,4,5'-Pentachlorobiphenyl - 2,2',4,5,5'-Pentachlorobiphenyl - 2,3,3',4',6-Pentachlorobiphenyl - 2,2',3,4,4',5'-Hexachlorobiphenyl - 2,2',3,4,5,5'-Hexachlorobiphenyl - 2,2',3,5,5',6-Hexachlorobiphenyl - 2,2',4,4',5,5'-Hexachlorobiphenyl - 2,2',3,3',4,4',5-Heptachlorobiphenyl - 2,2',3,4,4',5,5'-Heptachlorobiphenyl - 2,2',3,4,4',5,6-Heptachlorobiphenyl - 2,2',3,4',5,5',6-Heptachlorobiphenyl - 2,2',3,3',4,4',5,6-Nonachlorobiphenyl Pentachlorophenol	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[1,9,26] 2) Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method ^[10,26] 3) Automated Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method ^[11,26] Electrometric Method ^[23,24]
29	pH	
30	Selenium	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[1,6,16] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method ^[1,6,17] 3) Digestion, Inductively Coupled Plasma Method ^[7,16] 4) Digestion, Inductively Coupled Plasma/Mass Spectrometric Method ^[7,17]

31

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
31	Silver	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[1,6,16] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method ^[1,6,17] 3) Digestion, Inductively Coupled Plasma Method ^[7,16] 4) Digestion, Inductively Coupled Plasma/Mass Spectrometric Method ^[7,17]
32	Thallium	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[1,6,16] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method ^[1,6,17] 3) Digestion, Inductively Coupled Plasma Method ^[7,16] 4) Digestion, Inductively Coupled Plasma/Mass Spectrometric Method ^[7,17]
33	Toxaphene	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[1,9,26] 2) Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method ^[10,26] 3) Automated Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method ^[11,26]
34	Vanadium	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[1,6,16] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method ^[1,6,17] 3) Digestion, Inductively Coupled Plasma Method ^[7,16] 4) Digestion, Inductively Coupled Plasma/Mass Spectrometric Method ^[7,17]
35	Zinc	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[1,6,16] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method ^[1,6,17] 3) Digestion, Inductively Coupled Plasma Method ^[7,16] 4) Digestion, Inductively Coupled Plasma/Mass Spectrometric Method ^[7,17]

สมิ

ดิน จำนวน 125 รายการ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
1	Acenaphthene	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[11,26]
2	Acetone	1) Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[15,25] 2) Equilibrium Headspace, Gas Chromatographic/ Mass Spectrometric Method ^[13]
3	Aldrin	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[11,26]
4	Anthracene	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[11,26]
5	Antimony	1) Digestion, Inductively Coupled Plasma Method ^[7,16] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method ^[7,17]
6	Arsenic	1) Digestion, Inductively Coupled Plasma Method ^[7,16] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method ^[7,17]
7	Atrazine	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[11,26]
8	Barium	1) Digestion, Inductively Coupled Plasma Method ^[7,16] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method ^[7,17]
9	Benz(a)anthracene	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[11,26]
10	Benzene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[15,25]

sm

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
11	Benzo(b)fluoranthene	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[11,26]
12	Benzo(k)fluoranthene	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[11,26]
13	Benzoic acid	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[11,26]
14	Benzo(a)pyrene	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[11,26]
15	Benzo(g,h,i)perylene	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[11,26]
16	Beryllium	1) Digestion, Inductively Coupled Plasma Method ^[7,16] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method ^[7,17]
17	Bis(2-chloroethyl)ether	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[11,26]
18	Bis(2-ethylhexyl)phthalate	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[11,26]
19	Bromodichloromethane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[15,25]
20	Bromoform	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[15,25]
21	Butanol	Equilibrium Headspace, Gas Chromatographic/ Mass Spectrometric Method ^[13,25]
22	Butyl Benzyl Phthalate	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[11,26]

3mg

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
23	Cadmium	1) Digestion, Inductively Coupled Plasma Method ^[7,16] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method ^[7,17]
24	Carbazole	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[11,26]
25	Carbon Disulfide	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[15,25]
26	Carbon tetrachloride	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[15,25]
27	Chlordane	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[11,26]
28	p-Chloroaniline	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[11,26]
29	Chlorobenzene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[15,25]
30	Chlorodibromomethane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[15,25]
31	Chloroform	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[15,25]
32	2-Chlorophenol	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[11,26]
33	Chromium	1) Digestion, Inductively Coupled Plasma Method ^[7,16] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method ^[7,17]
34	Chromium (III)	1) Digestion, Inductively Coupled Plasma Method; Alkaline Digestion, Colorimetric Method; Calculation Method ^[7,8,16,19] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method; Alkaline Digestion, Colorimetric Method; Calculation Method ^[7,8,17,19]
35	Chromium (VI)	Alkaline Digestion, Colorimetric Method ^[8,19]



ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
36	Chrysene	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[11,26]
37	Cyanide	Extraction, Distillation, Colorimetric Method ^[27,28,29]
38	2,4-D	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[11,26]
39	DDD	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[11,26]
40	DDE	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[11,26]
41	DDT	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[11,26]
42	Dibenz(a,h)anthracene	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[11,26]
43	Di-n-Butyl Phthalate	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[11,26]
44	1,2-Dichlorobenzene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[15,25]
45	1,3-Dichlorobenzene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[15,25]
46	1,4-Dichlorobenzene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[15,25]
47	3,3-Dichlorobenzidine	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[11,26]
48	1,1-Dichloroethane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[15,25]

Small

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
49	1,2-Dichloroethane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[15,25]
50	1,1-Dichloroethylene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[15,25]
51	cis-1,2-Dichloroethylene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[15,25]
52	trans-1,2-Dichloroethylene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[15,25]
53	2,4-Dichlorophenol	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[11,26]
54	1,2-Dichloropropane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[15,25]
55	1,3-Dichloropropane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[15,25]
56	1,3-Dichloropropene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[15,25]
57	Dieldrin	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[11,26]
58	Diethyl Phthalate	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[11,26]
59	2,4-Dimethylphenol	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[11,26]
60	2,4-Dinitrophenol	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[11,26]
61	2,4-Dinitrotoluene	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[11,26]
62	2,6-Dinitrotoluene	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[11,26]

Signature

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
63	Di-n-Octyl Phthalate	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[11,26]
64	Endosulfan	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[11,26]
65	Endrin	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[11,26]
66	Ethylbenzene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[15,25]
67	Fluoranthene	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[11,26]
68	Fluorene	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[11,26]
69	Heptachlor	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[11,26]
70	Heptachlor epoxide	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[11,26]
71	Hexachlorobenzene	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[11,26]
72	Hexachloro-1,3-butadiene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[15,25]
73	n-Hexane	1) Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[15,25] 2) Equilibrium Headspace, Gas Chromatographic/ Mass Spectrometric Method ^[13]

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
74	α -HCH	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[11,26]
75	β -HCH	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[11,26]
76	γ -HCH	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[11,26]
77	Hexachlorocyclopentadiene	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[11,26]
78	Hexachloroethane	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[11,26]
79	Indeno(1,2,3-cd)pyrene	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[11,26]
80	Isophorone	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[11,26]
81	Lead	1) Digestion, Inductively Coupled Plasma Method ^[7,16] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method ^[7,17]
82	Manganese	1) Digestion, Inductively Coupled Plasma Method ^[7,16] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method ^[7,17]
83	Mercury	1) Digestion, Cold-Vapor Atomic Absorption Spectrometric Method ^[20] 2) Thermal Decomposition, Amalgamation, and Atomic Absorption Spectrophotometry ^[21] 3) Digestion, Cold-Vapor Atomic Fluorescence Spectrometric Method ^[30]

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
84	Methanol	1) Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[15,25] 2) Equilibrium Headspace, Gas Chromatographic/ Mass Spectrometric Method ^[13,25]
85	Methoxychlor	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[11,26]
86	Methyl Bromide	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[15,25]
87	Methylene Chloride	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[15,25]
88	2-methylphenol	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[11,26]
89	2-Methylnaphthalene	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[11,26]
90	Methyl tert-Butyl Ether	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[15,25]
91	Naphthalene	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[11,26]
92	Nickel	1) Digestion, Inductively Coupled Plasma Method ^[7,16] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method ^[7,17]
93	Nitrobenzene	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[11,26]
94	N-Nitrosodiphenylamine	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[11,26]
95	N-Nitrosodi-n-propylamine	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[11,26]

3/11/21

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
96	Polychlorinated biphenyls (PCBs) - Aroclor 1016 - Aroclor 1221 - Aroclor 1232 - Aroclor 1242 - Aroclor 1248 - Aroclor 1254 - Aroclor 1260 - 2-Chlorobiphenyl - 2,2',3,5'-Tetrachlorobiphenyl - 2,2',5,5'-Tetrachlorobiphenyl - 2,3',4,4'-Tetrachlorobiphenyl - 2,2',3,4,5'-Pentachlorobiphenyl - 2,2',4,5,5'-Pentachlorobiphenyl - 2,3,3',4',6-Pentachlorobiphenyl - 2,2',3,4,4',5'-Hexachlorobiphenyl - 2,2',3,4,5,5'-Hexachlorobiphenyl - 2,2',3,5,5',6-Hexachlorobiphenyl - 2,2',4,4',5,5'-Hexachlorobiphenyl - 2,2',3,3',4,4',5-Heptachlorobiphenyl - 2,2',3,4,4',5,5'-Heptachlorobiphenyl - 2,2',3,4,4',5,6-Heptachlorobiphenyl - 2,2',3,4',5,5',6-Heptachlorobiphenyl - 2,2',3,3',4,4',5,5',6-Nonachlorobiphenyl	1) Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method ^[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method ^[11,26]
97	Pentachlorophenol	1) Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method ^[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method ^[11,26]
98	Phenanthrene	1) Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method ^[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method ^[11,26]

สมย

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
99	Phenol	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[11,26]
100	Pyrene	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[11,26]
101	Selenium	1) Digestion, Inductively Coupled Plasma Method ^[7,16] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method ^[7,17]
102	Silver	1) Digestion, Inductively Coupled Plasma Method ^[7,16] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method ^[7,17]
103	Styrene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[15,25]
104	1,1,2,2-Tetrachloroethane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[15,25]
105	Tetrachloroethylene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[15,25]
106	Toluene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[15,25]
107	Toxaphene	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[11,26]
108	TPH (C ₅ -C ₈)	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[15,25]
109	TPH (C ₈ -C ₁₆)	1) Automate Extraction, Gas Chromatographic Method ^[11,22] 2) Solvent Extraction, Gas Chromatographic Method ^[12,22] 3) Ultrasonic Extraction, Gas Chromatographic Method ^[22,31]
110	TPH (C ₁₆ - C ₃₅)	1) Automate Extraction, Gas Chromatographic Method ^[11,22] 2) Solvent Extraction, Gas Chromatographic Method ^[12,22] 3) Ultrasonic Extraction, Gas Chromatographic Method ^[22,31]
111	1,2,4-Trichlorobenzene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[15,25]
112	1,1,1-Trichloroethane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[15,25]
113	1,1,2-Trichloroethane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[15,25]
114	Trichloroethylene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[15,25]

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
115	2,4,5-Trichlorophenol	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[11,26]
116	2,4,6-Trichlorophenol	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[11,26]
117	1,3,5-Trimethylbenzene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[15,25]
118	Vanadium	1) Digestion, Inductively Coupled Plasma Method ^[7,16] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method ^[7,17]
119	Vinyl Acetate	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[15,25]
120	Vinyl Chloride	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[15,25]
121	m-Xylene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[15,25]
122	o-Xylene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[15,25]
123	p-Xylene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[15,25]
124	Xylene (Total)	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[15,25]
125	Zinc	1) Digestion, Inductively Coupled Plasma Method ^[7,16] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method ^[7,17]

จกผ

เอกสารอ้างอิง

- กระทรวงอุตสาหกรรม. ประกาศกระทรวงอุตสาหกรรม, พ.ศ. 2566. เรื่อง การจัดการสิ่งปฏิกูลหรือวัสดุที่ไม่ใช้แล้ว. ราชกิจจานุเบกษา. 31 พฤษภาคม 2566. เล่มที่ 140 ตอนพิเศษ 126 ง.
- กระทรวงอุตสาหกรรม. ประกาศกระทรวงอุตสาหกรรม, พ.ศ. 2549. เรื่อง กำหนดค่าปริมาณเขม่าควันที่เจือปนในอากาศที่ระบายออกจากปล่องของหม้อน้ำโรงสีข้าวที่ใช้กลบเป็นเชื้อเพลิง. ราชกิจจานุเบกษา. 4 ธันวาคม 2549. เล่มที่ 123 ตอนพิเศษ 125ง.
- สมาคมวิศวกรรมสิ่งแวดล้อมแห่งประเทศไทย. คู่มือวิเคราะห์น้ำเสีย. พิมพ์ครั้งที่ 4. กรุงเทพฯ: เรือนแก้วการพิมพ์, 2547.
- APHA, AWWA, WEF. Standard Methods for the Examination of Water and Wastewater. 24th ed. Washington, DC: APHA, 2023.

5. United States Environmental Protection Agency. **Standards of Performance for New Stationary Sources**. 40 CFR 60. Appendix A, 2023.

6. United States Environmental Protection Agency. **Test Methods for Evaluating Solid Waste Physical/Chemical Methods**. SW-846, 2014.

7. United States Environmental Protection Agency. **Test Methods for Evaluating Solid Waste Physical/Chemical Methods. Acid Digestion of Sludges and Sediments and Soils**. SW-846 Method 3050B, 1996.

8. United States Environmental Protection Agency. **Test Methods for Evaluating Solid Waste Physical/Chemical Methods. Alkaline Digestion for Hexavalent Chromium**. SW-846 Method 3060A, 1996.

9. United States Environmental Protection Agency. **Test Methods for Evaluating Solid Waste Physical/Chemical Methods. Separatory Funnel Liquid-Liquid Extraction**. SW-846 Method 3510C, 1996.

10. United States Environmental Protection Agency. **Test Methods for Evaluating Solid Waste Physical/Chemical Methods. Soxhlet Extraction**. SW-846 Method 3540C, 1996.

11. United States Environmental Protection Agency. **Test Methods for Evaluating Solid Waste Physical/Chemical Methods. Automated Soxhlet Extraction**. SW-846 Method 3541, 1994.

12. United States Environmental Protection Agency. **Test Methods for Evaluating Solid Waste Physical/Chemical Methods. Microscale Solvent Extraction (MSE)**. SW-846 Method 3570, 2002.

13. United States Environmental Protection Agency. **Test Methods for Evaluating Solid Waste Physical/Chemical Methods. Volatile Organic Compounds (VOCs) in Various Sample Matrices Using Equilibrium Headspace Analysis**. SW-846 Method 5021A, 2014.

14. United States Environmental Protection Agency. **Test Methods for Evaluating Solid Waste Physical/Chemical Methods. Purge-and-Trap for Aqueous Samples**. SW-846 Method 5030B, 1996.

15. United States Environmental Protection Agency. **Test Methods for Evaluating Solid Waste Physical/Chemical Methods. Closed-System Purge-and-Trap and Extraction for Volatile Organics in Soil and Waste Samples**. SW-846 Method 5035, 1996.

16. United States Environmental Protection Agency. **Test Methods for Evaluating Solid Waste Physical/Chemical Methods. Inductively Coupled Plasma-Atomic Emission Spectrometry**. SW-846 Method 6010B, 1996.

17. United States Environmental Protection Agency. **Test Methods for Evaluating Solid Waste Physical/Chemical Methods. Inductively Coupled Plasma-Mass Spectrometry**. SW-846 Method 6020A, 2007.

18. United States Environmental Protection Agency. **Test Methods for Evaluating Solid Waste Physical/Chemical Methods. Antimony and Arsenic (Atomic Absorption, Borohydride Reduction)**. SW-846 Method 7062, 1994. **เพิ่มใหม่**

19. United States Environmental Protection Agency. **Test Methods for Evaluating Solid Waste Physical/Chemical Methods. Chromium, Hexavalent (Colorimetric)**. SW-846 Method 7196A, 1992. **เพิ่มใหม่**

20. United States...

20. United States Environmental Protection Agency. Test Methods for Evaluating Solid Waste Physical/Chemical Methods. Mercury in Solid or Semisolid Waste (Manual Cold-Vapor Technique). SW-846 Method 7471B, 2007.

21. United States Environmental Protection Agency. Test Methods for Evaluating Solid Waste Physical/Chemical Methods. Mercury in Solids and Solutions by Thermal Decomposition, Amalgamation, and Atomic Absorption Spectrophotometry. SW-846 Method 7473, 2007.

22. United States Environmental Protection Agency. Test Methods for Evaluating Solid Waste Physical/Chemical Methods. Nonhalogenated Organics by Gas Chromatography. SW-846 Method 8015C, 2007.

23. United States Environmental Protection Agency. Test Methods for Evaluating Solid Waste Physical/Chemical Methods. pH Electrometric Measurement. SW-846 Method 9040C, 2004.

24. United States Environmental Protection Agency. Test Methods for Evaluating Solid Waste Physical/Chemical Methods. Soil and Waste pH. SW-846 Method 9045D, 2004.

25. United States Environmental Protection Agency. Test Methods for Evaluating Solid Waste Physical/Chemical Methods. Volatile Organic Compounds by Gas Chromatography/Mass Spectrometry (GC/MS). SW-846 Method 8260D, 2018.

26. United States Environmental Protection Agency. Test Methods for Evaluating Solid Waste Physical/Chemical Methods. Semivolatile Organic Compounds by Gas Chromatography/Mass Spectrometry (GC/MS). SW-846 Method 8270E, 2018.

27. United States Environmental Protection Agency. Test Methods for Evaluating Solid Waste Physical/Chemical Methods. Total and Amenable Cyanide: Distillation SW-846 Method 9010B, 1996.

28. United States Environmental Protection Agency. Test Methods for Evaluating Solid Waste Physical/Chemical Methods. Cyanide Extraction Procedure for Solids and Oil. SW-846 Method 9013A, 1996.

29. United States Environmental Protection Agency. Test Methods for Evaluating Solid Waste Physical/Chemical Methods. Cyanide in Waters and Extracts Using Titrimetric and Manual Spectrophotometric Procedures. SW-846 Method 9014, 2014.

30. United States Environmental Protection Agency. Test Methods for Evaluating Solid Waste Physical/Chemical Methods. Mercury in Sediment and Tissue Samples by Atomic Fluorescence Spectrometry. SW-846 Method 7474, 2007.

31. United States Environmental Protection Agency. Test Methods for Evaluating Solid Waste Physical/Chemical Methods. Ultrasonic Extraction. SW-846 Method 3550C, 2007.

Sign

ที่ ออก ๐๓๑๐(๑)/ ๔๑ ๒๑



กรมโรงงานอุตสาหกรรม
ถนนพระรามที่ ๖ แขวงทุ่งพญาไท
เขตราชเทวี กรุงเทพฯ ๑๐๔๐๐

๒๕ เมษายน ๒๕๖๗

เรื่อง เปลี่ยนแปลงบุคลากรของห้องปฏิบัติการวิเคราะห์

เรียน กรรมการผู้จัดการ บริษัท เอแอลเอส แลบลอราทอรี กรุ๊ป (ประเทศไทย) จำกัด

อ้างถึง คำขอขึ้นทะเบียน/ต่ออายุ/เปลี่ยนแปลงบุคลากร และชนิดสารมลพิษของห้องปฏิบัติการวิเคราะห์เอกชน
ลงวันที่ ๒๙ มีนาคม ๒๕๖๗

ตามคำขอที่อ้างถึง บริษัท เอแอลเอส แลบลอราทอรี กรุ๊ป (ประเทศไทย) จำกัด ห้องปฏิบัติการวิเคราะห์เอกชน เลขทะเบียน ว-๒๐๔ สถานที่ตั้งเลขที่ ๑๐๔ ซอยพัฒนาการ ๔๐ ถนนพัฒนาการ แขวงพัฒนาการ เขตสวนหลวง กรุงเทพมหานคร ขอเปลี่ยนแปลงบุคลากร ความละเอียดแจ้งแล้ว นั้น

กรมโรงงานอุตสาหกรรมพิจารณาแล้ว มีความเห็นดังนี้

๑. ให้ยกเลิกเจ้าหน้าที่ประจำห้องปฏิบัติการวิเคราะห์ จำนวน ๓ ราย

- | | |
|--------------------------|----------------------------|
| ๑) นางสาวพรรณธิดา พุ่มคง | ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๖๕ |
| ๒) นายกำชัย สุทธิระ | ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๒๑ |
| ๓) นางสาวศุภรดา ปันมยุรา | ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๓๘ |

๒. ให้เพิ่มเจ้าหน้าที่ห้องปฏิบัติการวิเคราะห์เอกชน จำนวน ๑๒ ราย

- | | |
|-----------------------------|----------------------------|
| ๑) นางสาวฐานิดา กลิ่นเขียว | ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๘๒ |
| ๒) นางสาวกัญญ์ภัสสร สายคำ | ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๘๓ |
| ๓) นางสาวณัฐนันท์ กันทะวงศ์ | ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๘๔ |
| ๔) นายอำนาจ วงษาเคน | ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๘๕ |
| ๕) นายกฤษณพล ปัญญาวงศ์ | ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๘๖ |
| ๖) นายณชากร หารรรษา | ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๘๗ |
| ๗) นายวัชรินทร์ ผ่องสามสวน | ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๘๘ |
| ๘) นายณัฐพงศ์ โสภาก | ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๘๙ |
| ๙) นายศักรินทร์ ปานเพ็ง | ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๙๐ |
| ๑๐) นายณัฐพล ชุ่มชื่น | ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๙๑ |
| ๑๑) นายธนา สุพาพันธุ์ | ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๙๒ |
| ๑๒) นายนราธร แก้วพงษ์ชา | ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๙๓ |

อนึ่ง หนังสือฉบับนี้...

อนึ่ง หนังสือฉบับนี้จะหมดอายุพร้อมหนังสือต่ออายุรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน
ในวันที่ ๒ กันยายน ๒๕๖๙

จึงเรียนมาเพื่อทราบ

ขอแสดงความนับถือ



(นายพรยศ กลั่นกรอง)

รองอธิบดี ปฏิบัติราชการแทน

อธิบดีกรมโรงงานอุตสาหกรรม

กองวิจัยและเตือนภัยมลพิษโรงงาน

กลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษและทะเบียนห้องปฏิบัติการ

โทร. ๐ ๒๔๓๐ ๖๓๑๒ ต่อ ๒๑๐๓-๕

โทรสาร ๐ ๒๔๓๐ ๖๓๑๒ ต่อ ๒๑๙๙

ไปรษณีย์อิเล็กทรอนิกส์ saraban@diw.mail.go.th





ที่ อก ๐๓๑๐(๑)/ ๑๒๓๖ ๘ /

กรมโรงงานอุตสาหกรรม
ถนนพระรามที่ ๖ แขวงทุ่งพญาไท
เขตราชเทวี กรุงเทพฯ ๑๐๔๐๐

๑๘ ธันวาคม ๒๕๖๗

เรื่อง ยกเลิกบุคลากรของห้องปฏิบัติการวิเคราะห์

เรียน กรรมการผู้จัดการ บริษัท เอแอลเอส แลบบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด

อ้างถึง คำขอขึ้นทะเบียน/ต่ออายุ/เปลี่ยนแปลงบุคลากร และชนิดสารมลพิษของห้องปฏิบัติการวิเคราะห์เอกชน
ลงวันที่ ๒ ธันวาคม ๒๕๖๗

ตามคำขอที่อ้างถึง บริษัท เอแอลเอส แลบบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด ห้องปฏิบัติการ
วิเคราะห์เอกชน เลขทะเบียน ว-๒๐๔ สถานที่ตั้งเลขที่ ๑๐๔ ซอยพัฒนาการ ๔๐ ถนนพัฒนาการ แขวงพัฒนาการ
เขตสวนหลวง กรุงเทพมหานคร ขอยกเลิกบุคลากร ความละเอียดแจ้งแล้ว นั้น

กรมโรงงานอุตสาหกรรมพิจารณาแล้ว ให้ยกเลิกเจ้าหน้าที่ประจำห้องปฏิบัติการวิเคราะห์
จำนวน ๘ ราย ได้แก่

- | | |
|-------------------------------|----------------------------|
| ๑) นายประพจน์ วรรณชูชัย | ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๖๐ |
| ๒) นายจิรณัฐ ขวละอ | ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๗๒ |
| ๓) นายพีรพัฒน์ กำคำ | ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๐๘ |
| ๔) นางสาวอริยา คำคลอง | ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๓๔ |
| ๕) นายกิตติพงศ์ แซ่ลี | ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๔๔ |
| ๖) นายจิรเมธ ประเสริฐศิริพงศ์ | ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๖๐ |
| ๗) นายภัทรพงษ์ มณฑาทอง | ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๖๗ |
| ๘) นางสาวจารุวรรณ กระจำงพันธ์ | ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๘๑ |

จึงเรียนมาเพื่อทราบ

ขอแสดงความนับถือ

(นายธีรทัศน์ อิศรางกูร ณ อยุธยา)

รองอธิบดี ปฏิบัติราชการแทน
อธิบดีกรมโรงงานอุตสาหกรรม

กองวิจัยและเตือนภัยมลพิษโรงงาน

กลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษและทะเบียนห้องปฏิบัติการ

โทร. ๐ ๒๔๓๐ ๖๓๑๒ ต่อ ๒๑๐๓-๕

โทรสาร ๐ ๒๔๓๐ ๖๓๑๒ ต่อ ๒๑๙๙

ไปรษณีย์อิเล็กทรอนิกส์ saraban@diw.mail.go.th



“อุตสาหกรรมก้าวไกล ประเทศไทยก้าวหน้า ร่วมกันพัฒนา อุตสาหกรรมสีเขียว”





ที่ อก ๐๓๑๐(๑)/ ๓ ๑ ๕ ๐

กรมโรงงานอุตสาหกรรม
ถนนพระรามที่ ๖ แขวงทุ่งพญาไท
เขตราชเทวี กรุงเทพฯ ๑๐๕๐๐

๑๐ เมษายน ๒๕๖๘

เรื่อง ยกเลิกบุคลากรของห้องปฏิบัติการวิเคราะห์

เรียน กรรมการผู้จัดการ บริษัท เอแอลเอส แลบบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด

อ้างถึง คำขอขึ้นทะเบียน/ต่ออายุ/เปลี่ยนแปลงบุคลากร และชนิดสารมลพิษของห้องปฏิบัติการวิเคราะห์เอกชน
ลงวันที่ ๒ เมษายน ๒๕๖๘

ตามคำขอที่อ้างถึง บริษัท เอแอลเอส แลบบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด ห้องปฏิบัติการ
วิเคราะห์เอกชน เลขทะเบียน ว-๒๐๔ สถานที่ตั้งเลขที่ ๑๐๔ ซอยพัฒนาการ ๔๐ ถนนพัฒนาการ แขวงพัฒนาการ
เขตสวนหลวง กรุงเทพมหานคร ขอยกเลิกบุคลากร ความละเอียดแจ้งแล้ว นั้น

กรมโรงงานอุตสาหกรรมพิจารณาแล้ว ให้ยกเลิกเจ้าหน้าที่ประจำห้องปฏิบัติการวิเคราะห์
จำนวน ๒ ราย ได้แก่

๑) นายธิตินพงศ์ บัวแดง

ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๐๒

๒) นายมงคล ผลาทิพย์

ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๑๐

จึงเรียนมาเพื่อทราบ

ขอแสดงความนับถือ

(นายธีรทัศน์ อิศรางกูร ณ อยุธยา)

รองอธิบดี ปฏิบัติราชการแทน

อธิบดีกรมโรงงานอุตสาหกรรม

กองวิจัยและเตือนภัยมลพิษโรงงาน

กลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษและทะเบียนห้องปฏิบัติการ

โทร. ๐ ๒๔๓๐ ๖๓๑๒ ต่อ ๒๑๐๓-๕

โทรสาร ๐ ๒๔๓๐ ๖๓๑๒ ต่อ ๒๑๙๙

ไปรษณีย์อิเล็กทรอนิกส์ saraban@diw.mail.go.th



ที่ อก ๐๓๑๐(๑)/ ๔ ๖ ๗ ๓



กรมโรงงานอุตสาหกรรม
ถนนพระรามที่ ๖ แขวงทุ่งพญาไท
เขตราชเทวี กรุงเทพฯ ๑๐๔๐๐

๐ ๕ มิถุนายน ๒๕๖๔

เรื่อง เปลี่ยนแปลงบุคลากรของห้องปฏิบัติการวิเคราะห์

เรียน กรรมการผู้จัดการ บริษัท เอแอลเอส แลบบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด

อ้างถึง คำขอขึ้นทะเบียน/ต่ออายุ/เปลี่ยนแปลงบุคลากร และชนิดสารมลพิษของห้องปฏิบัติการวิเคราะห์เอกชน
ลงวันที่ ๗ พฤษภาคม ๒๕๖๔

ตามคำขอที่อ้างถึง บริษัท เอแอลเอส แลบบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด ห้องปฏิบัติการ
วิเคราะห์เอกชน เลขทะเบียน ว-๒๐๔ สถานที่ตั้งเลขที่ ๑๐๔ ซอยพัฒนาการ ๔๐ ถนนพัฒนาการ แขวงพัฒนาการ
เขตสวนหลวง กรุงเทพมหานคร ขอเปลี่ยนแปลงบุคลากร ความละเอียดแจ้งแล้ว นั้น

กรมโรงงานอุตสาหกรรมพิจารณาแล้ว ให้เพิ่มเจ้าหน้าที่ห้องปฏิบัติการวิเคราะห์เอกชน
จำนวน ๑๑ ราย ได้แก่

- | | |
|-----------------------------------|----------------------------|
| ๑) นายคุณากร มั่นชื่น | ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๙๔ |
| ๒) นายชัยมงคล แสนมาตร | ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๙๕ |
| ๓) นายเอกรินทร์ บุตส์กิติ | ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๙๖ |
| ๔) นายพัชชานนท์ อินปรีก | ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๙๗ |
| ๕) นายศตวรรษ แก้วกันหา | ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๙๘ |
| ๖) นายวิกรม มีศิริ | ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๙๙ |
| ๗) นายภคินันท์ คำจันทราช | ทะเบียนเลขที่ ว-๒๐๔-จ-๐๒๐๐ |
| ๘) นายศิริวิทย์ มีไพฑูรย์ | ทะเบียนเลขที่ ว-๒๐๔-จ-๐๒๐๑ |
| ๙) นายธีรพงษ์ ศรีคำแหง | ทะเบียนเลขที่ ว-๒๐๔-จ-๐๒๐๒ |
| ๑๐) นายอภิสิทธิ์ ศรีคงแก้ว | ทะเบียนเลขที่ ว-๒๐๔-จ-๐๒๐๓ |
| ๑๑) ว่าที่ร้อยตรี ภาณุพงศ์ แสนศรี | ทะเบียนเลขที่ ว-๒๐๔-จ-๐๒๐๔ |

อนึ่ง หนังสือฉบับนี้จะสิ้นอายุพร้อมหนังสือต่ออายุรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน
ในวันที่ ๒ กันยายน ๒๕๖๔

จึงเรียนมาเพื่อทราบ

ขอแสดงความนับถือ

(นายธีระ จันท์เกิด)

นักวิทยาศาสตร์เชี่ยวชาญ รักษาราชการแทน
ผู้อำนวยการกองวิจัยและเตือนภัยมลพิษโรงงาน
ปฏิบัติราชการแทนอธิบดีกรมโรงงานอุตสาหกรรม

กองวิจัยและเตือนภัยมลพิษโรงงาน

กลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษและทะเบียนห้องปฏิบัติการ

โทร. ๐ ๒๔๓๐ ๖๓๑๒ ต่อ ๒๑๐๓-๕

โทรสาร ๐ ๒๔๓๐ ๖๓๑๒ ต่อ ๒๑๙๙

ไปรษณีย์อิเล็กทรอนิกส์ saraban@diw.mail.go.th



“อุตสาหกรรมก้าวไกล ประเทศไทยก้าวหน้า ร่วมกันพัฒนา อุตสาหกรรมสีเขียว”





๐๘ สิงหาคม ๒๕๖๗

เรื่อง ต่ออายุหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน

เรียน กรรมการผู้จัดการ บริษัท เอแอลเอส แลบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด

อ้างถึง คำขอขึ้นทะเบียน/ต่ออายุ/เปลี่ยนแปลงบุคลากร และชนิดสารมลพิษของห้องปฏิบัติการวิเคราะห์เอกชน ลงวันที่ ๒๗ พฤษภาคม ๒๕๖๗

สิ่งที่ส่งมาด้วย เอกสารแนบท้ายหนังสือต่ออายุรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน บริษัท เอแอลเอส แลบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด จำนวน ๓ แผ่น

ตามคำขอที่อ้างถึง บริษัท เอแอลเอส แลบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด ขอต่ออายุหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน เลขทะเบียน ว-๓๒๓ สถานที่ตั้งเลขที่ ๖๑๖/๑๐ หมู่ที่ ๕ ตำบลแม่ น้ำคู้ อำเภอลพบุรี จังหวัดระยอง ต่อกรมโรงงานอุตสาหกรรม นั้น

กรมโรงงานอุตสาหกรรมพิจารณาแล้ว ให้บริษัท เอแอลเอส แลบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด ต่ออายุหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน โดยมีองค์ประกอบดังนี้

ก. ผู้ควบคุมห้องปฏิบัติการวิเคราะห์เอกชน

- | | |
|--------------------------|----------------------------|
| ๑) นายเดช ช้างชน | ทะเบียนเลขที่ ว-๓๒๓-ค-๐๐๐๑ |
| ๒) นางวิลาวัลย์ บริรักษ์ | ทะเบียนเลขที่ ว-๓๒๓-ค-๐๐๐๒ |
| ๓) นายสุพจน์ สลามเต๊ะ | ทะเบียนเลขที่ ว-๓๒๓-ค-๐๐๐๓ |

ข. เจ้าหน้าที่ห้องปฏิบัติการวิเคราะห์เอกชน

- | | |
|--------------------------------|----------------------------|
| ๑) นายณัฐพงษ์ เพ็งขาวนา | ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๐๑ |
| ๒) นางสาวกัลยพรรณ รักษ์ดี | ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๐๒ |
| ๓) นางสาวจุฑารัตน์ สีสองกลาง | ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๐๓ |
| ๔) นางสาวจิตสุภา ประเทืองสุข | ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๐๔ |
| ๕) นายสรสรเสริญ ค่อยยกสุข | ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๐๕ |
| ๖) นายณัฐวุฒิ อภมพรมราช | ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๐๖ |
| ๗) นายจิตรกร สีวะสา | ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๐๗ |
| ๘) นายสิทธิพิชญ์ สุวรรณรัตน์ | ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๐๘ |
| ๙) นายสิทธิพันธ์ เสนาชีวะ | ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๐๙ |
| ๑๐) นายอนุเวศน์ เตมา | ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๑๐ |
| ๑๑) นายสุรวิทย์ นราพงษ์ | ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๑๑ |
| ๑๒) นายณัฐพล เจริญวรวงศ์ | ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๑๓ |
| ๑๓) นายชานนท์ บุญชื่น | ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๑๔ |
| ๑๔) นายณัฐกานต์ วงศ์อินทร์อยู่ | ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๑๕ |
| ๑๕) นายอานนท์ โพธิ์พระทอง | ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๑๖ |

๑๖) นายณัฏพล...

๑๖) นายณัฏฐพล ถ้ำกลาง
๑๗) นายศุภณัฐ พิสัยพันธ์
๑๘) นายวสันต์ คินันติ
๑๙) นายวรัญญู ฉิมพาลี
๒๐) นายศุภณัฐ สกฤติตติมศักดิ์
๒๑) นายเอกชัย ถันทอง
๒๒) นายพงษ์เทพ สิทธิเลาะ
๒๓) นายทินกร กุมภาชี
๒๔) นางสาวนันทยา เบญจจันทร์
๒๕) นายสิทธิชัย ยันพิมาย
๒๖) นางสาวปภาณิน หลอดทอง
๒๗) นางสาวพจนา สีดา
๒๘) นางสาวธนิศา กุลศิริวงศ์
๒๙) นายพิทยา ทองแดง
๓๐) นางสาวชลธิชา สุนงกษ
๓๑) ว่าที่ร้อยตรี รณชัย ม่วงมา
๓๒) นายวรารุณ ฟ้าพา
๓๓) นายศักดิ์รินทร์ จรัสกาย
๓๔) นายสุรศักดิ์ สาชิน
๓๕) นายสถาพร ถาแก้ว
๓๖) นายสุทธิดำรง โชคปิตินันท์
๓๗) นายวัลลภ หันไชยเนาว์
๓๘) นางสาววนาลี เจริญตระกูล
๓๙) นายชนะสิทธิ์ วงศ์ไชย
๔๐) นายชัยนุสรณ์ เลิศนันทกุลชัย
๔๑) นายสัจจา เพ็ชรแสง
๔๒) นายกัณตภณ มณีสัมพันธ์
๔๓) นายธารินทร์ อ็อกจินดา
๔๔) นายศุภชัย วงศ์สุริย์ฉาย
๔๕) นายไสว ตันโพธิ์
๔๖) นางสาวกิตติยา สัญญาอริยาภรณ์
๔๖) นางสาวธิดารัตน์ ศิริมังคะโร
๔๗) นายพิพัฒน์ นิภัทร์เศรษฐ์
๔๘) นายศิริวิทย์ เรืองสม
๔๙) นายปารเมศ สัตยาคุณ
๕๐) นายณนฎนาท ธรรมสระโร
๕๑) นางสาวศุภรัตน์ โสจันทร์

ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๑๗
ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๑๘
ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๑๙
ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๒๐
ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๒๑
ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๒๒
ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๒๓
ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๒๔
ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๒๕
ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๒๖
ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๒๗
ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๒๘
ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๒๙
ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๓๐
ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๓๑
ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๓๒
ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๓๓
ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๓๔
ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๓๕
ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๓๖
ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๓๗
ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๓๘
ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๓๙
ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๔๐
ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๔๑
ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๔๒
ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๔๓
ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๔๔
ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๔๕
ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๔๖
ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๔๗
ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๔๘
ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๔๙
ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๕๐
ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๕๑
ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๕๒
ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๕๓

๕๒) นายพชรกร...

๕๒) นายพชรกร เจ็งเจริญ	ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๕๔
๕๓) นายทิวากร เชื้อมาก	ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๕๕
๕๔) นายอนุรักษ ทองขจรศักดิ์	ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๕๖
๕๕) นายอภิชาติ วิลาศ	ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๕๗
๕๖) นายจรัสระวี ศรีรักษา	ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๕๘
๕๘) นายประสานมิตร เชื้อนเพชร	ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๕๙
๕๙) นายภาณุวัฒน์ วังบง	ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๖๐
๖๐) นายสันติ ชัยชนะ	ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๖๑
๖๑) นายทินกร กุลชาติ	ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๖๒

ค. ขอบข่ายชนิดสารมลพิษที่ได้รับขึ้นทะเบียนให้วิเคราะห์ในน้ำเสีย น้ำใต้ดิน อากาศเสีย ตามสิ่งที่ส่งมาด้วย

หนังสือฉบับนี้จะหมดอายุในวันที่ ๒๘ มิถุนายน ๒๕๗๑ หากประสงค์จะต่ออายุหนังสือ รับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน ให้ยื่นคำขอต่ออายุพร้อมเอกสารประกอบคำขอต่อกรมโรงงานอุตสาหกรรมภายใน ๖๐ วัน ก่อนวันสิ้นอายุของหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน

จึงเรียนมาเพื่อทราบ

ขอแสดงความนับถือ



(นายพยศ กลั่นกรอง)

รองอธิบดี ปฏิบัติราชการแทน
อธิบดีกรมโรงงานอุตสาหกรรม

ศูนย์วิจัยและเตือนภัยมลพิษโรงงานภาคตะวันออก

โทร. ๐ ๓๓๑๓ ๖๐๕๙ ต่อ ๕๐๐๑-๒

ไปรษณีย์อิเล็กทรอนิกส์ airw@diw.mail.go.th



“อุตสาหกรรมก้าวไกล ประเทศไทยก้าวหน้า ร่วมกันพัฒนา อุตสาหกรรมสีเขียว”



เอกสารแนบท้ายหนังสือเปลี่ยนแปลงสารมลพิษของห้องปฏิบัติการวิเคราะห์เอกชน
บริษัท เอแอลเอส แลборาทอรี กรุ๊ป (ประเทศไทย) จำกัด เลขทะเบียน ว-๓๒๓
ที่ อก ๐๓๒๐/ ๗ ๙ ๓ ๘ ลงวันที่ ๐๘ สิงหาคม ๒๕๖๗

ขอข่ายสารมลพิษที่ได้รับขึ้นทะเบียนจากกรมโรงงานอุตสาหกรรม จำนวน ๒๔ รายการ
น้ำเสีย จำนวน 14 รายการ

ลำดับ ที่	สารมลพิษ	วิธีวิเคราะห์
1	Biochemical Oxygen Demand	1) 5-Day BOD Test, Membrane Electrode Method ^[2] 2) 5-Day BOD Test, Azide Modification Method ^[2]
2	Chemical Oxygen Demand	1) Open Reflux, Titrimetric Method ^[2] 2) Closed Reflux, Colorimetric Method ^[2] 3) Closed Reflux, Titrimetric Method ^[2]
3	Color	ADMI Weighted-Ordinate Spectrophotometric Method ^[2]
4	Cyanide	Distillation, Colorimetric Method ^[2]
5	Formaldehyde	Distillation, Colorimetric Method ^[1]
6	Free Chlorine	DPD Ferrous Titrimetric Method ^[2]
7	Oil and Grease	Liquid-Liquid, Partition-Gravimetric Method ^[2]
8	pH	Electrometric Method ^[2]
9	Phenols	1) Distillation, Chloroform Extraction Method ^[2] 2) Distillation, Direct Photometric Method ^[2]
10	Sulfide	ZnS Precipitation, Iodometric Method ^[2]
11	Temperature	Field Method ^[2]
12	Total Dissolved Solids	Dried at 180 °C ^[2]
13	Total Kjeldahl Nitrogen	Semi-Macro Kjeldahl Method ^[2]
14	Total Suspended Solids	Dried at 103-105 °C ^[2]

น้ำใต้ดิน จำนวน 3 รายการ

ลำดับ ที่	สารมลพิษ	วิธีวิเคราะห์
1	Cyanide	Distillation, Colorimetric Method ^[2]
2	pH	Electrometric Method ^[2]
3	Phenols	Distillation, Direct Photometric Method ^[2]

อากาศเสีย...

อากาศเสีย (ปล่อยระบาย) จำนวน 7 รายการ

ลำดับ ที่	สารมลพิษ	วิธีวิเคราะห์
1	Carbon Monoxide	1) Sampling Bag, Non-Dispersive Infrared Method ^[5] 2) Instrumental Analyzer Method ^[9]
2	Hydrogen Sulfide	Absorption Sampling, Iodometric Method ^[5]
3	Opacity	Ringelmann's Method ^[3,4]
4	Oxide of Nitrogen	1) Absorption Sampling, Phenoldisulfonic Acid Method ^[8] 2) Instrumental Analyzer Method ^[10]
5	Sulfur Dioxide	1) Absorption Sampling, Barium-Thorin Titrimetric Acid Method ^[5] 2) Instrumental Analyzer Method ^[11]
6	Sulfuric Acid	Isokinetic Sampling, Barium – Titrimetric Method ^[6]
7	Total Suspended Particulate	Isokinetic Sampling, Gravimetric Method ^[7]

เอกสารอ้างอิง

1. ธงชัย พรรณสวัสดิ์ และวิบูลย์ลักษณ์ วิสุมิศักดิ์, บรรณาธิการ. (2547) คู่มือวิเคราะห์น้ำเสีย. พิมพ์ครั้งที่ 4. กรุงเทพฯ: สมาคมวิศวกรรมสิ่งแวดล้อมแห่งประเทศไทย.
2. APHA, AWWA, WEF. **Standard Methods for the Examination of Water and Wastewater**. 24th ed. Washington, DC : APHA, 2023
3. กระทรวงอุตสาหกรรม. ประกาศกระทรวงอุตสาหกรรม, พ.ศ. 2549. เรื่อง กำหนดค่าปริมาณเขม่าควันที่เจือปนในอากาศที่ระบายออกจากปล่องของหม้อน้ำโรงสีข้าวที่ใช้กลบเป็นเชื้อเพลิง. ราชกิจจานุเบกษา. 4 ธันวาคม 2549. เล่มที่ 123 ตอนพิเศษ 125ง
4. กระทรวงอุตสาหกรรม. ประกาศกระทรวงอุตสาหกรรม, พ.ศ. 2549. เรื่อง กำหนดค่าปริมาณเขม่าควันที่เจือปนในอากาศที่ระบายออกจากปล่องของหม้อน้ำของโรงงาน. ราชกิจจานุเบกษา. 4 ธันวาคม 2549. เล่มที่ 123 ตอนพิเศษ 125ง
5. United States Environmental Protection Agency. **Standards of Performance for New Stationary Sources**. 40 CFR 60. Appendix A, 2017.
6. United States Environmental Protection Agency. **Standards of Performance for New Stationary Sources**. 40 CFR 60. Appendix A, 2019.
7. United States...

7. United States Environmental Protection Agency. Standards of Performance for New Stationary Sources. 40 CFR 60. Appendix A, 2020.

8. United States Environmental Protection Agency. Standards of Performance for New Stationary Sources. 40 CFR 60. Appendix A, 2023.

9. United States Environmental Protection Agency. Determination of Carbon Monoxide Emission from Stationary Sources; Instrumental Analyzer Procedure. 40 CFR 60. Appendix A Method 10, 2017.

10. United States Environmental Protection Agency. Determination of Oxide of Nitrogen Emission from Stationary Sources; Instrumental Analyzer Procedure. 40 CFR 60. Appendix A Method 7E, 2023.

11. United States Environmental Protection Agency. Determination of Sulfur dioxide Emission from Stationary Sources; Instrumental Analyzer Procedure. 40 CFR 60. Appendix A Method 6C, 2017.

A handwritten signature in black ink, consisting of a large, stylized 'O' followed by a horizontal line and a short vertical stroke.

ที่ อก ๐๓๒๐/ ๑๐๐๙ ๙



กรมโรงงานอุตสาหกรรม
ถนนพระรามที่ ๖ แขวงทุ่งพญาไท
เขตราชเทวี กรุงเทพฯ ๑๐๔๐๐

๐๔ ตุลาคม ๒๕๖๗

เรื่อง แกไขรายชื่อเจ้าหน้าที่ห้องปฏิบัติการวิเคราะห์เอกชน

เรียน กรรมการผู้จัดการ บริษัท เอแอลเอส แลבורาทอรี กรุ๊ป (ประเทศไทย) จำกัด

อ้างถึง หนังสือ บริษัท เอแอลเอส แลבורาทอรี กรุ๊ป (ประเทศไทย) จำกัด เลขที่ Env 2024/005
ลงวันที่ ๓๐ สิงหาคม ๒๕๖๗

ตามหนังสือที่อ้างถึง บริษัท เอแอลเอส แลבורาทอรี กรุ๊ป (ประเทศไทย) จำกัด ห้องปฏิบัติการวิเคราะห์เอกชน เลขทะเบียน ว-๓๒๓ สถานที่ตั้งเลขที่ ๖๑๖/๑๐ หมู่ที่ ๕ ตำบลแม่น้ำคู้ อำเภอลวกแดง จังหวัดระยอง ขอแก้ไขชื่อเจ้าหน้าที่ห้องปฏิบัติการวิเคราะห์เอกชน เนื่องจากมีความคลาดเคลื่อน ความละเอียดแจ้งแล้ว นั้น

กรมโรงงานอุตสาหกรรม ได้รับทราบและดำเนินการแก้ไขรายชื่อเจ้าหน้าที่ห้องปฏิบัติการวิเคราะห์เอกชน จำนวน ๕ ราย ตามที่แจ้งเรียบร้อยแล้ว เป็นดังนี้

ลำดับที่ ๒๗ นางพจนา สีดา

ลำดับที่ ๒๘ นางสาวธนิดา กุลสุริวงศ์

ลำดับที่ ๓๐ นางชลธิชา สุปงกช

ลำดับที่ ๓๖ นายสุทธิดำรงค์ โชคปิตินันท์

ลำดับที่ ๔๒ นายกันตภณ มณีสัมพันธ์

จึงเรียนมาเพื่อทราบ

ขอแสดงความนับถือ

น

(นายพรยศ กลิ่นกรอง)

รองอธิบดี ปฏิบัติราชการแทน
อธิบดีกรมโรงงานอุตสาหกรรม

ศูนย์วิจัยและเตือนภัยมลพิษโรงงานภาคตะวันออก

โทร. ๐ ๓๓๑๓ ๖๐๕๙ ต่อ ๕๐๐๑-๒

ไปรษณีย์อิเล็กทรอนิกส์ eirw@diw.mail.go.th



“อุตสาหกรรมก้าวไกล ประเทศไทยก้าวหน้า ร่วมกันพัฒนา อุตสาหกรรมสีเขียว”



ที่ อก ๐๓๑๐(๓)/ ๕ ๒ ๔ ๖



กรมโรงงานอุตสาหกรรม
ถนนพระรามที่ ๖ แขวงทุ่งพญาไท
เขตราชเทวี กรุงเทพฯ ๑๐๔๐๐

๒๐ พฤษภาคม ๒๕๖๘

เรื่อง ยกเลิกบุคลากรของห้องปฏิบัติการวิเคราะห์

เรียน กรรมการผู้จัดการ บริษัท เอแอลเอส แลบบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด

อ้างถึง คำขอขึ้นทะเบียน/ต่ออายุ/เปลี่ยนแปลงบุคลากร และชนิดสารมลพิษของห้องปฏิบัติการวิเคราะห์เอกชน
ลงวันที่ ๑๐ เมษายน ๒๕๖๘

ตามคำขอที่อ้างถึง บริษัท เอแอลเอส แลบบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด ห้องปฏิบัติการวิเคราะห์เอกชน เลขทะเบียน ว-๓๒๓ สถานที่ตั้งเลขที่ ๖๑๖/๑๐ หมู่ที่ ๕ ตำบลแม่น้ำคู้ อำเภอปลวกแดง จังหวัดระยอง ขอยกเลิกบุคลากร ความละเอียดแจ้งแล้ว นั้น

กรมโรงงานอุตสาหกรรมพิจารณาแล้ว ให้ยกเลิกเจ้าหน้าที่ห้องปฏิบัติการวิเคราะห์เอกชน จำนวน ๑ ราย ได้แก่ นายปารเมศ สัตยาคุณ ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๕๑

จึงเรียนมาเพื่อทราบ

ขอแสดงความนับถือ

(นายประสม ดำรงพงษ์)

ผู้อำนวยการกองวิจัยและเตือนภัยมลพิษโรงงาน
ปฏิบัติราชการแทนอธิบดีกรมโรงงานอุตสาหกรรม

ศูนย์วิจัยและเตือนภัยมลพิษโรงงานภาคตะวันออก

โทร. ๐ ๓๓๑๓ ๖๐๕๕ ต่อ ๕๐๐๑-๒

ไปรษณีย์อิเล็กทรอนิกส์ eirw@diw.mail.go.th



“อุตสาหกรรมก้าวไกล ประเทศไทยก้าวหน้า ร่วมกันพัฒนา อุตสาหกรรมสีเขียว”



ที่ อก ๐๓๑๐(๓)/ ๕๕๐๙



กรมโรงงานอุตสาหกรรม

ถนนพระรามที่ ๖ แขวงทุ่งพญาไท

เขตราชเทวี กรุงเทพฯ ๑๐๕๐๐

๒๗ พฤษภาคม ๒๕๖๘

เรื่อง เปลี่ยนแปลงชื่อ-สกุลบุคลากรของห้องปฏิบัติการวิเคราะห์

เรียน กรรมการผู้จัดการ บริษัท เอแอลเอส แลบบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด

อ้างถึง คำขอขึ้นทะเบียน/ต่ออายุ/เปลี่ยนแปลงบุคลากร และชนิดสารมลพิษของห้องปฏิบัติการวิเคราะห์เอกชน
ลงวันที่ ๑๕ พฤษภาคม ๒๕๖๘

ตามคำขอที่อ้างถึง บริษัท เอแอลเอส แลบบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด ห้องปฏิบัติการวิเคราะห์เอกชน เลขทะเบียน ว-๓๒๓ สถานที่ตั้งเลขที่ ๖๑๖/๑๐ หมู่ที่ ๕ ตำบลแม่ น้ำคู้ อำเภอปลวกแดง จังหวัดระยอง ขอเปลี่ยนแปลงชื่อ-สกุลบุคลากร ความละเอียดแจ้งแล้ว นั้น

กรมโรงงานอุตสาหกรรมพิจารณาแล้ว ให้เปลี่ยนแปลงชื่อ-สกุลบุคลากร จำนวน ๑ ราย
จากนายธนະสิทธิ์ วงศ์ไชย เป็น นายอมลวิทย์ วงศ์ไชย

จึงเรียนมาเพื่อทราบ

ขอแสดงความนับถือ

(นายประสม ดำรงพงษ์)

ผู้อำนวยการกองวิจัยและเตือนภัยมลพิษโรงงาน
ปฏิบัติราชการแทนอธิบดีกรมโรงงานอุตสาหกรรม

ศูนย์วิจัยและเตือนภัยมลพิษโรงงานภาคตะวันออก

โทร. ๐ ๓๓๑๓ ๖๐๕๙ ต่อ ๕๐๐๑-๒

ไปรษณีย์อิเล็กทรอนิกส์ eirw@diw.mail.go.th



“อุตสาหกรรมก้าวไกล ประเทศไทยก้าวหน้า ร่วมกันพัฒนา อุตสาหกรรมสีเขียว”





right solutions.
right partner.

✉ bangkok@alsglobal.com



ALS Line Official
ID: @alsthailand



ALS Facebook
Search: ALS Thailand