ภาคผนวก ง

เอกสารการสอบเทียบเครื่องมือตรวจวิเคราะห์

right solutions.
right partner.


รายการเครื่องมือที่ใช้ในการวิเคราะห์ / ทดสอบ

Sample Name	Parameter	Equipment Name	ID No.	Calibrated Date	Next Cal	Freq. Calibrate (Months)
Ambient	Carbon Monoxide	CO Analyzer	BKK_FS0790	2-Jan-25	2-Jul-25	6
Ambient	Nitrogen Dioxide	NO_2 Analyzer	BKK_FS0789	3-Jan-25	3-Jul-25	6
Ambient	Total Hydrocarbon	THC Analyzer	BKK_FS0805	2-Jan-25	2-Jul-25	6
Ambient	Total Suspended Particulate	High Volume	BKK_FS0369	-	-	On site Calibration
Ambient	Total Suspended Particulate	Digital Balance	BKK_EN0403	3-Jun-24	3-Jun-25	12
Ambient	Particulate Matter (PM-10)	High Volume	BKK_FS0389	-	-	On site Calibration
Ambient	Particulate Matter (PM-10)	Digital Balance	BKK_EN0403	3-Jun-24	3-Jun-25	12
Ambient	Wind Speed / Wind Direction	Wind Speed / Wind Direction	BKK_FS0163	1-Apr-25	1-Oct-26	18
Noise	Leq 24 hrs	Sound Calibrator	BKK_FS1221	10-Jan-25	10-Jan-26	12
Noise	Leq 24 hrs	Sound Level Meter	BKK_FS0099	30-Aug-24	30-Aug-25	12
Water Lab	Settleable Solids	Chamber (Cooling Room)	BKK_EN0167	4-Jun-25	4-Dec-26	18
Water Lab	Sulfide	Burette	BKK_EN0171	27-Feb-24	27-Aug-25	18
Water Lab	Sulfide	Chamber (Cooling Room)	BKK_EN0167	4-Jun-25	4-Dec-26	18
Water Lab	pH at 25 °C	pH meter	BKK_EN0342	17-Oct-24	17-Oct-25	12
Water Lab	Oil & Grease	Electronic Top-Loading Balance	BKK_EN0003	2-Aug-24	2-Aug-25	12
Water Lab	Oil & Grease	Water Bath	BKK_EN0439	29-Oct-24	29-Oct-25	12
Water Lab	Total Kjeldahl Nitrogen	Digestion Unit	BKK_EN0366	9-Apr-25	9-Apr-26	12
Water Lab	Total Kjeldahl Nitrogen	Discrete analyzer	BKK_EN0037	16-Aug-24	16-Aug-25	12
Water Lab	Total Suspended Solids	Electronic Top-Loading Balance	BKK_EN0003	2-Aug-24	2-Aug-25	12
Water Lab	Total Suspended Solids	Oven	BKK_EN0273	14-May-24	14-Nov-25	18
Water Lab	Total Dissolved Solids 180°C	Electronic Top-Loading Balance	BKK_EN0003	2-Aug-24	2-Aug-25	12
Water Lab	Total Dissolved Solids 180°C	Oven	BKK_EN0273	14-May-24	14-Nov-25	18
Water Lab	BOD	DO Meter	BKK_EN0017	20-May-25	20-Nov-26	18
Water Lab	BOD	Incubator	BKK_EN0304	4-Mar-25	4-Mar-26	12
Water Lab	BOD	Burette	BKK_EN0171	27-Feb-24	27-Aug-25	18
Water Lab	Total Coliform	Autoclave	BKK_ML0041	4-Mar-25	4-Sep-26	18
Water Lab	Total Coliform	Incubator	BKK_ML0010	3-Dec-24	3-Dec-25	12
Water Lab	Total Coliform	Hot Air Oven	BKK_ML0013	23-Apr-24	23-Oct-25	18
Water Lab	Fecal Coliform	Autoclave	BKK_ML0041	4-Mar-25	4-Sep-26	18
Water Lab	Fecal Coliform	Incubator	BKK_ML0010	3-Dec-24	3-Dec-25	12
Water Lab	Fecal Coliform	Hot Air Oven	BKK_ML0013	23-Apr-24	23-Oct-25	18
Water Lab	Fecal Coliform	Water Bath	BKK_ML0056	4-Mar-25	4-Mar-26	12
Water Lab	*Escherichia coli*	Autoclave	BKK_ML0041	4-Mar-25	4-Sep-26	18
Water Lab	*Escherichia coli*	Incubator	BKK_ML0010	3-Dec-24	3-Dec-25	12
Water Lab	*Escherichia coli*	Hot Air Oven	BKK_ML0013	23-Apr-24	23-Oct-25	18
Water Lab	*Escherichia coli*	Water Bath	BKK_ML0056	4-Mar-25	4-Mar-26	12
Water Lab	Ammonium	Discrete analyzer	BKK_EN0037	16-Aug-24	16-Aug-25	12
Water Lab	Total Alkalinity	Burette	BKK_EN0171	27-Feb-24	27-Aug-25	18
Water Lab	Calcium Hardness	Burette	BKK_EN0171	27-Feb-24	27-Aug-25	18
Water Lab	Residual Free Chlorine	Chlorine Meter	BKK_LG0040	13-Aug-24	13-Aug-25	12
Water Lab	Residual Chlorine	Chlorine Meter	BKK_LG0040	13-Aug-24	13-Aug-25	12
Water Lab	Nitrate	Ion Chromatography	BKK_EN0069	12-Jan-24	12-Jul-25	18
Water Lab	Chloride	Ion Chromatography	BKK_EN0069	12-Jan-24	12-Jul-25	18
Water Lab	Cyanuric acid	Spectrophotometer	SGK_CL0100	25-Dec-24	25-Dec-25	12

MULTIPOINT CALIBRATION REPORT

Calibration Date	2-Jan-25	**Equipment Name**	CO Analyzer
Manufacturer	HORIBA	**Model**	APMA-370
Serial No.	SLWK5D7G	**Equipment ID**	BKK_FS0790
Calibrator Manufacturer	Teledyne API	**Model**	700
Serial No.	947		
Std. Gas Concentration (PPM)	55.22	**Cylinder No.**	GN0027222
Cylinder Pressure (psi)	1800	**Certified By**	Airgas Inc.
Certified Date	9-Feb-22	**Expired Date**	9-Feb-30

Point	CALIBRATION RESULTS			
	Ideal	Actual	Error	%Error
ZERO	0.00	0.10	0.10	0.10
1	100.00	98.50	-1.50	-1.50
2	200.00	198.60	-1.40	-0.70
3	300.00	298.30	-1.70	-0.57
4	400.00	397.80	-2.20	-0.55
AVERAGE (%)				-0.64

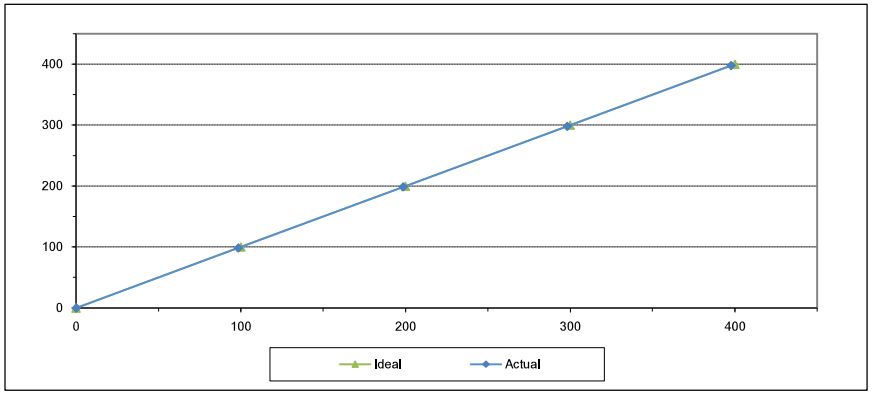

Calibrated By

(Mr.Jirawut Sakarn)
Field Environmental Scientist (3)


Approved By

(Mr.Sarayuth Jittranont)
Assistant General Manager

MULTIPOINT CALIBRATION REPORT

Calibration Date	3-Jan-25	Equipment Name	NOx Analyzer
Manufacturer	HORIBA	Model	APNA-370
Serial No.	R26E09EW	Equipment ID	BKK_FS0789
Calibrator Manufacturer	Teledyne API	Model	700
Serial No.	947		
Std. Gas Concentration (PPM)	55.88	Cylinder No.	GN0027222
Cylinder Pressure (psi)	1800	Certified By	Airgas Inc.
Certified Date	9-Feb-22	Expired Date	9-Feb-30

Point	CALIBRATION RESULTS						
	Ideal	Actual NO	Error NO	%Error NO	Actual NOx	Error NOx	%Error NOx
ZERO	0.00	0.10	0.10	0.10	0.10	0.10	0.10
1	100.00	99.00	-1.00	-1.00	101.10	1.10	1.10
2	200.00	198.30	-1.70	-0.85	201.10	1.10	0.55
3	300.00	298.50	-1.50	-0.50	302.20	2.20	0.73
4	400.00	398.60	-1.40	-0.35	398.50	-1.50	-0.38
AVERAGE (%)				-0.52			0.42

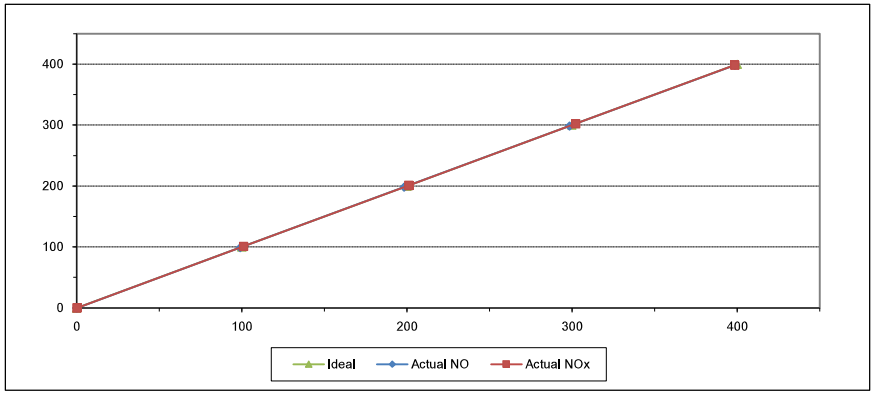

Calibrated By

(Mr.Jirawut Sakarn)
Field Environmental Scientist (3)


Approved By

(Mr.Sarayuth Jittranont)
Assistant General Manager

MULTIPOINT CALIBRATION REPORT

Calibration Date	2-Jan-25	Equipment Name	THC Analyzer
Manufacturer	HORIBA	Model	APHA-370
Serial No.	C4BHPA0H	Equipment ID	BKK_FS0805
Calibrator Manufacturer	Teledyne API	Model	700
Serial No.	947		
Std. Gas Conc. (PPM C3H8)	50.9	Cylinder No.	D612257
Cylinder Pressure (psi)	1800	Certified By	Linde
Certified Date	27-Jun-18	Expired Date	27-Jun-26

Point	CALIBRATION RESULTS			
	Ideal	Autual	Error	%Error
ZERO	0.00	0.10	0.10	0.10
1	100.00	98.90	-1.10	-1.10
2	200.00	199.20	-0.80	-0.40
3	300.00	298.30	-1.70	-0.57
4	400.00	396.90	-3.10	-0.78
AVERAGE (%)				-0.55

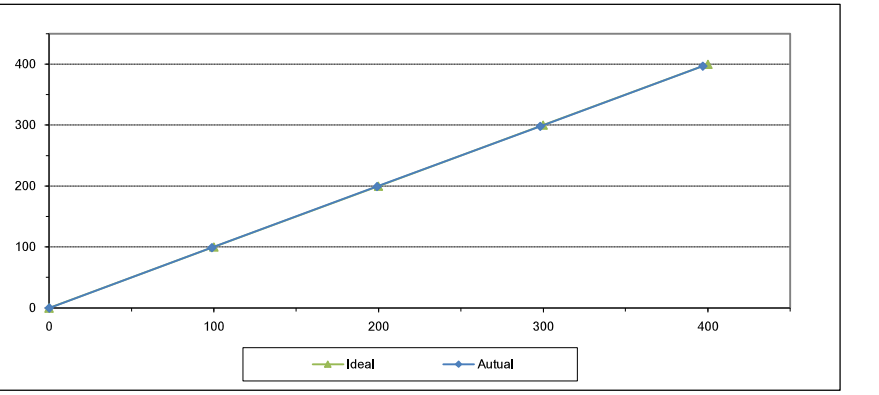

Calibrated By

(Mr.Jirawut Sakarn)
Field Environmental Scientist (3)


Approved By

(Mr.Sarayuth Jittranont)
Assistant General Manager

High Volume Air Sampler Calibration Worksheet

Project Site :	One Sukhumvit 59 Company Limited	**Barometric Pressure (mm Hg) :**	757.2
Calibrate Location :	บริเวณพื้นที่โครงการ	**Temperature (°C) :**	36
Calibrate Date :	6-May-25	**High Volume ID :**	BKK_FS0369
CalibrationSheet No.:	C-060525-BKK_FS0369	**High Volume Model :**	TE-5009X
Calibrator ID:	BKK_FS0625	**High Volume S/N :**	4166
Calibrator Model :	TE-5028A	**Calibrator Slope :**	1.67329
Calibrator S/N :	2585	**Calibrator Intercept :**	-0.01925

Test No.	Delta H_2O (inch)	Q_{std} (m^3/min)	I : Chart (CFM)	Linear Regression	
1	3.2	1.0672	40	Slope :	44.7432
2	3.8	1.1612	46	Intercept :	-6.8474
3	4.6	1.2757	50	Correlation Coefficient :	0.9930
4	5.4	1.3805	56		
5	6.5	1.5128	60		

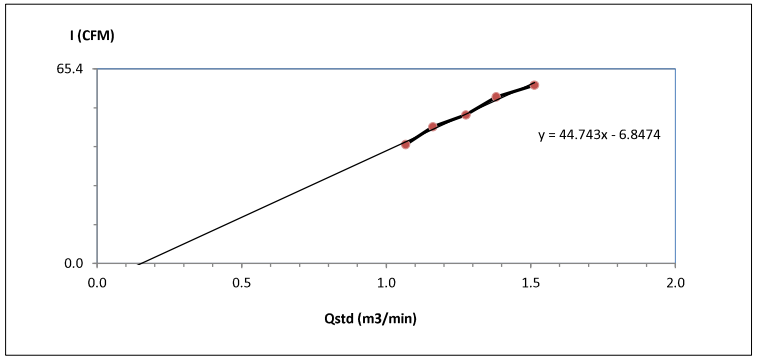

Calibrated by _____

(Mr. Prommee Sripatnet)
Field Services Scientist (2)

Approved by : _____

(Mr. Noppong Juntarupan)
BKK Field Coordinator Scientist (3)

FORM NO.: F 06-073 REVISION NO.:2 ISSUE DATE: 20/11/23

PLAY SOLUTION TECHNOLOGY COMPANY LIMITED
179/75 Nawong Pradit Pattana Road, 3 Ban, Dannuang, Nonthaburi 11210
Tel.+662 011 0505, Fax+662 010 2702
www.playsolutec.com

NSC-TISI-TISI17025 CALIBRATION 0370

CERTIFICATE OF CALIBRATION

Certificate No. : PST-0126-24 W/O No. : WO-0053-24

Page no. 1 of 3

Customer

Company : ALS LABORATORY GROUP (THAILAND) CO., LTD.
Address : 104 Phatthanakan 40, Phatthanakan Road, Khwaeng Phatthanakan,
City / Province : Khet Suan Luang, Bangkok
Zip/Postal : 10250

Device

Equipment : Electronic Balance Capacity 110 / 210 g
Manufacturer : OHAUS Readability 0.00001 / 0.0001 g
Model : EX225D/AD ID No. BKK_EN0435
Serial No. : C309774648
Condition : Normal

Environment Conditions

Location of Calibration : Environment Lab
Ambient Temperature : 30.1 (°C) ± 3 °C
Relative Humidity : 70.3 (%RH) ± 15 %RH
Barometric Pressure : 1011.3 (mbar) ± 10 hPa
Comment :

REVIEW BY Siruda K.
APPROVED BY Siriluk P.
NEXT CAL. DATE 03/06/25

Date of Receipt : June 3, 2024
Date of Calibration : June 3, 2024
Issue Date : June 5, 2024

Calibrated by : Mr.Kittichai Rattanatham
Calibrator

Approved by : Mr. Kittichai Rattanatham
Approved Signature

The reported measurement result relates only to the measured and applies only at the time of measurement.

This Certificate is issued in accordance with the conditions of accreditation granted by Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and is traceability to recognize national standards and to the unit of measurement realized at the corresponding national standard laboratory. This certificate may not be reproduced other than in full except with the prior written approval prior written approval of the calibration center, Play Solution Technology Co.,Ltd

PLAY SOLUTION TECHNOLOGY COMPANY LIMITED
179/75 Nawong Prachai Pattana Road, Sikan, Donmuang, Bangkok 10210
Tel.:+66 2 011 0505, Fax:+66 2 010 7720
www.playsolution.com

NSC-TISI-TIST7025
CALIBRATION 0078

CERTIFICATE OF CALIBRATION

Certificate No. : PST-0126-24 W/O No. : WO-0051-24

Result of Calibration : Without Adjustment

1. Repeatability

Weighing Range 1 g	Nominal Value g	Standard Deviation g
Max capacity 220	50	0.000013
	200	0.000048

2.Linearity; Departure of Indication from nominal Value

Weighing Range 1

Nominal Value g	Standard Value g	Indication g	Error of Indication g	Expanded Uncertainty g	Factor k
0.01	0.01000	0.01000	-0.000001	0.000082	2.87
0.1	0.10001	0.10001	0.000004	0.000082	2.87
0.5	0.50000	0.50001	0.000013	0.00008	2.87
1	1.00001	1.00002	0.000013	0.00008	2.87
5	5.00002	5.00003	0.000009	0.00008	2.52
10	9.99999	9.99998	-0.000001	0.00008	2.18
50	50.00001	49.99998	-0.000027	0.00016	2.00
100	100.00003	100.00002	0.000004	0.00030	2.00
150	150.00003	150.0001	0.000077	0.00045	2.00
200	200.00003	200.0001	0.000058	0.00060	2.00

PLAY SOLUTION TECHNOLOGY COMPANY LIMITED
179/75 Nawong Prachai Pattana Road, Sikan, Donmuang, Bangkok 10210
Tel.:+66 2 011 0505, Fax:+66 2 010 7720
www.playsolution.com

NSC-TISI-TIST7025
CALIBRATION 0078

CERTIFICATE OF CALIBRATION

Certificate No. : PST-0126-24 W/O No. : WO-0051-24

Result of Calibration

3.Eccentricity

Test load at least 1/3 of the maximum capacity, typically placed between 1/2 and 1/3 of the distance from the centre of the load receptor to the edge.



☑ ☐

Weighing Range 1
Test Load : 100 g

Position	Indication g
1	100.00004
2	100.00005
3	100.00003
4	100.00004
5	100.00003
Max. Deviation	0.00002

Standard method

The calibration was performed by using calibration laboratory's in-house calibration method : CP-M-001 based on "LILAS LAB 14 Calibration of weighing machine" : edition 6 | October 2019

Reference standards instrument

Instrument	OIML Class	S/N	Certificate No.	Due Date
Standard Weight Set	E2	4000021852	22-128725	November 30, 2024
Standard Weight Set	-	-	-	-
Standard Weight Set	-	-	-	-
Standard Weight Set	-	-	-	-

Measurement Uncertainty

The given measurement uncertainty is the standard of the measurement multiplied by the coverage factor k which corresponds to a confidence level of about 95%, for a normal distribution. The standard uncertainty was calculated according to LILAS M3003.


Traceability: The measurement is traceable to national standard, which realize the physical unit of measurement (SI) Through the reference calibration laboratory of Asia Medical and Agricultural Laboratory and Research Center Co.,Ltd

END OF REPORT

High Volume Air Sampler Calibration Worksheet

Project Site :	One Sukhumvit 59 Company Limited	**Barometric Pressure (mm Hg) :**	757.2
Calibrate Location :	บริเวณพื้นที่โครงการ	**Temperature (°C) :**	36
Calibrate Date :	6-May-25	**High Volume ID :**	BKK_FS0389
CalibrationSheet No.:	**C-060525-BKK_FS0389**	**High Volume Model :**	TE-5009X
Calibrator ID:	BKK_FS0625	**High Volume S/N :**	5329
Calibrator Model :	TE-5028A	**Calibrator Slope :**	1.04803
Calibrator S/N :	2585	**Calibrator Intercept :**	-0.01206

Test No.	Delta H_2O (inch)	Qa (m^3/min)	I : Chart (CFM)	Linear Regression	
1	2.2	0.916	32	Slope :	35.1477
2	2.8	1.032	36	Intercept :	-0.3357
3	3.6	1.169	40	Correlation Coefficient :	0.9973
4	4.1	1.246	44		
5	5.0	1.375	48		

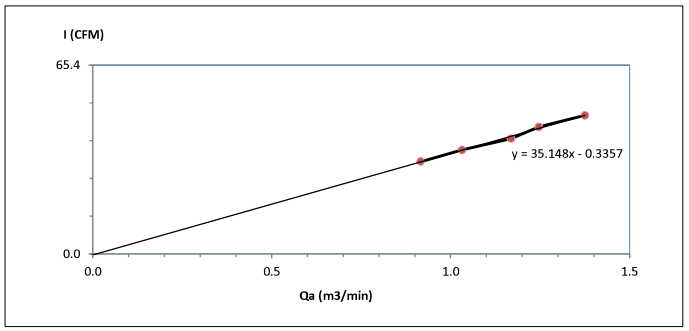

Calibrated by _____ Approved by : _____

(Mr. Prommee Sripatnet)
Field Services Scientist (2)

(Mr. Noppong Juntarupan)
BKK Field Coordinator Scientist (3)

FORM NO.: F 06-074 REVISION NO.:2 ISSUE DATE: 20/11/23

JIRANATEE ASSOCIATES CO.,LTD.

Accredited calibration laboratory
ISO/IEC 17025:2017
NSC-TISI-TIS 17025
CALIBRATION 0367

Recognized measurement laboratory
Calibration services department.

NSC – TISI – TIS 17025
CALIBRATION 0367

Certificate Number
C/VS-009-68

CERTIFICATE OF CALIBRATION

Page 1 of 2 Pages

MEASUREMENT ITEM	: Cup anemometer
MANUFACTURER	: Novalynx
MODEL/TYPE	: Sensor: WS-02F Data logger: 200-WS-25LB
SERIAL NUMBER	: Sensor: WSD-AM917 Data logger: A4917
ID NUMBER	: BKK_FS0163
CONDITION AS-RECEIVED	: Used item
CUSTOMER	: ALS laboratory group (Thailand) Co., Ltd. 104 Phatthanakan 43, Phatthanakan Rd, Khwaeng Suan Luang, Khet Suan Luang, Bangkok 10250 Thailand.
RECEIVED DATE	: 14 Mar 2025
MEASUREMENT DATE	: 01 Apr 2025
ISSUE DATE	: 01 Apr 2025

ENVIRONMENTAL CONDITIONS:
Ambient condition in the laboratory are as follow:

Temperature	: 23.0 ± 3.0	°C
Relative Humidity	: 55.0 ± 15.0	%RH
Atmospheric Pressure	: 1010± 10	hPa

PLACE OF CALIBRATION : Eiffel-type wind tunnel of Jiranatee Associates Co., Ltd.

CALIBRATION CONDITIONS

Wind tunnel cross-section area[1]	900	cm^2
Cup anemometer frontal area[2]	100	cm^2
Diameter of mounting pipe[3]	-	mm
Blockage ratio of test object[4]	0.111	(-)

Preconditioning : 24 hours at ambient conditions.
Measurement Condition : The average values during measurement are (25.0) °C, (42.6) %RH and (1012.1) hPa.

TABULATION OF RESULTS:
The table on next page give the measured values.

Calibrated by:
☒ Mr. Sorawit Tiwakitti
☐ Miss Jittrapan Boonyarit

Approved signatory

Mr. Parinya Noncharoen
Calibration Department Manager

Calibration procedure:
The Cup anemometer was calibrated against Standard air velocity transducer model: LSS-3.2 and pitot tube with precision differential pressure meter model: DPM2500 in an close test section of Eiffel-type wind tunnel with 900 cm^2 cross test section area. The IN-CL-062 based on IEC 61400-12-1, Wind energy generation systems – Part 12-1: Power performance measurements of electricity producing wind turbines, March 2017 was used as calibration guideline.

Traceability:
This certificate provides a traceability of The measurement to recognized the national standards, and to realization of the International system of Units (SI) through the NIMT (National Metrology Institute of Thailand) via Certificate number: MW-0097-24 and MW-0065-24

Uncertainty of Measurement:
The reported uncertainty of measurement is based on the standard uncertainty multiplied by a coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty has been determined in accordance with the GUM 'Evaluation of measurement data – Guide to the expression of uncertainty in measurement'

REVIEW BY .....
APPROVED BY .....
NEXT CAL DATE ..... 01/10/26 .....

Remark:
[1] Nozzle cross-section area of the wind tunnel
[2] Projected cross-section area of the tested object include mounting pipe
[3] Diameter of mounting pipe
[4] Ratio [2] to [1]

THIS CERTIFICATE OF CALIBRATION MAY NOT BE REPRODUCED EXCEPT IN FULL UNLESS PERMISSION FOR REPRODUCTION HAS BEEN OBTAINED IN WRITING FROM THE LABORATORY

Certificate Number
CWS-009-68

MEASUREMENT RESULTS [5]

The Cup anemometer, Unit Under Calibration (UUC) wasexercise at 10 m/s for 5 mirutes prior to calibration being performed. The standard air velocity 0.5 m/s to 5 m/s was calculated by a standard air velocity transducer which was installed 50 mm away from wind tunnel nozzle and installed 40 mm away from top of the test section and the standard air velocity 5 m/s to 30 m/s was calculated by a pitot tube with precision differential pressure meter which was installed 50 mm away from wind tunnel nozzle and installed 40 mm away from top of the test section, UUC was mounted on a round vertical tube of the lower plate at center of test section. The calibration was carried out under both rising and falling air velocity in the range of 1 m/s to 15 m/s at calibration interval of 1 m/s. The results of calibration and associated measurement uncertainties are reported in the table below.

v_{std} [6] (m/s)	Temp. wind tunnel (°C)	Temp. room (°C)	v_{uuc} [7] (m/s)	Error (m/s)	U (k=2) (m/s)
1.014	24.88	25.00	0.9	-0.1	0.31
2.223	24.98	25.00	2.0	-0.2	0.31
3.053	24.72	25.00	3.0	-0.1	0.31
4.254	24.76	25.00	4.1	-0.2	0.31
4.96	24.76	25.00	5.0	0.0	0.31
5.98	24.70	25.00	6.0	0.0	0.31
7.02	24.80	25.00	7.1	0.1	0.31
7.95	24.70	25.00	8.1	0.1	0.31
9.01	24.80	25.00	9.2	0.2	0.31
10.00	24.80	25.00	10.1	0.1	0.31
11.05	24.90	25.00	11.2	0.1	0.32
12.04	25.00	25.00	12.2	0.2	0.31
13.01	24.90	25.00	13.1	0.1	0.31
14.01	24.92	25.00	14.2	0.2	0.31
15.08	24.80	25.00	15.4	0.3	0.31
16.00	24.84	25.00	16.3	0.3	0.31

Remark:

[5] Calibration results only count for the tested circumstances and environmental conditions during which calibration took place

[6] Velocity of standard

[7] Velocity of Unit Under Calibration

PHOTO OF CALIBRATION SET-UP



Calibration set-up of the Cup anemometer calibration in the wind tunnel of Jiranatee Associates Co., Ltd. The Cup anemometer shown may differ from the calibrated one. Remark: The proportion of the set-up is not true to scale due to imaging geometry.

End of Certificate of Calibration

JNAC JIRANATEE ASSOCIATES CO.,LTD

Jiranatee Associates Co.,Ltd.
68/14-15, 67/35-36
Pitchkasem 7,7/1 Rd. Watthapra, Bangkoknoi,
Bangkok 10600 (Thailand)
Tel: +66(0)840813
Mobile: +66883999453
E-mail: jnac-calibration@jiranatee.com
Web site: www.jiranatee.com

Accredited calibration laboratory
ISO/IEC 17025:2017
NSC-TISI-TIS 17025
CALIBRATION 0367

Wind direction measurement laboratory
Calibration services department

NSC – TISI – TIS 17025
CALIBRATION 0367

Certificate Number
CWS-009-68

CERTIFICATE OF CALIBRATION

MEASUREMENT ITEM : Wind Direction Sensor
MANUFACTURER : Nevalynx
MODEL/TYPE : Sensor: WS-02F
Data logger: 20C-WS-25L8
SERIAL NUMBER : Sensor: WSD-A4917
Data logger: A4517
ID NUMBER : BKK_FS0163
CONDITION AS-RECEIVED : Used item
CUSTOMER : AIS laboratory group (Thailand) Co., Ltd.
104 Phatthanakan 40, Phatthanakan Rd, Khwaeng Suan Luang, Khet Suan Luang, Bangkok 10250 Thailand.

RECEIVED DATE : 14 Mar 2025
MEASUREMENT DATE : 01 Apr 2025
ISSUE DATE : 01 Apr 2025

ENVIRONMENTAL CONDITIONS:
Ambient condition in the laboratory are as follow:

Temperature	: 23.0 ± 3.0	°C
Relative Humidity	: 55.0 ± 15.0	%RH
Atmospheric Pressure	: 1010 ± 10	hPa

PLACE OF CALIBRATION : Eiffel-type wind tunnel of Jiranatee Associates Co., Ltd.

CALIBRATION CONDITION

: Wind tunnel cross-section area[1]	900	cm^2
Wind direction frontal area[2]	129	cm^2
Dameter of mounting pipe[3]	-	mm
Blockage ratio of test object[4]	0.143	[-]

Preconditioning : 24 hours at ambient conditions.
Measurement Condition : The average values during measurement are (24.2)°C, (44.6) %RH and (1010.1) hPa.

TABULATION OF RESULTS:
The table on next page give the measured values.

Calibrated by:
☑ Mr. Sorawit Thachalad
☐ Miss Jittiporn Tertkamphol

JNAC JIRANATEE ASSOCIATES CO.,LTD

Approved signatory
Mr. Parinya Booncharoen
Calibration Department Manager

Calibration procedure:
The wind direction sensor was calibrated against Standard Rotary Encoder model: AX3009TS-DM04-P3-S-LI01 in an close test-section of Eiffel-type wind tunnel with 900 cm^2 cross test section area. The WI-CL-008 based on IEC 61400-12-1, Wind energy generation systems – Part 12-1: Power performance measurements of electricity producing wind turbines, March 2017 was used as a calibration guideline.

Traceability:
This certificate provides a traceability of The measurement to recognized the national standards, and to realization of the International system of units (SI) through the NIMT (National Metrology Institute of Thailand) via Certificate number: DA-0027-24.

Uncertainty of Measurement:
The reported uncertainty of measurement is based on the standard uncertainty multiplied by a coverage factor k=2, Which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty has been determined in accordance with the GUM 'Evaluation of measurement data - Guide to the expression of uncertainty in measurement'

Remark:
[1] Nozzle cross-section area of the wind tunnel
[2] Projected cross-section area of the tested object include mounting pipe
[3] Diameter of mounting pipe
[4] Ratio [2] to [1]

THIS CERTIFICATE OF CALIBRATION MAY NOT BE REPRODUCED EXCEPT IN FULL UNLESS PERMISSION FOR REPRODUCTION HAS BEEN OBTAINED IN WRITING FROM THE LABORATORY

Jiranatee Associates Co., Ltd.

Certificate Number
CAL-105-58

MEASUREMENT RESULTS [1]

The wind direction sensor was calibrated against standard rotary encoder by comparison method. During calibration, the measurement was carried out at 45° intervals in clockwise and counterclockwise direction after offset adjustment has been made. The flow speed of wind tunnel (usually 5 m/s) is kept constant while the sensor is rotated around its vertical axis. The results of calibration and associated measurement uncertainties are reported in the table below.

Air speed	D'_{av}	D'_{acc}	Error	U (k=2)
m/s	Degree (°)	Degree (°)	Degree (°)	Degree (°)
	45.000	41	-4	0.80
	90.000	86	-4	0.80
	135.000	130	-5	0.80
5.31	180.000	176	-4	0.80
	225.000	227	2	0.80
	270.000	275	5	0.80
	315.000	321	6	0.80
	360.000	358	-2	0.80

Remarks:

[1] Calibration results only valid for the tested circumstances environmental conditions during which calibration took place

[2] Direction of standard

[3] Direction of Unit Under Calibration

End of Certificate of Calibration

Jiranatee Associates Co., Ltd.

SITHIPORN ASSOCIATES CO., LTD.
CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand
Tel. +66 2433 8331 Email : calibration@sithiphorn.com

Cert. No. : ACC25002
Pages : 1 of 3

Calibration Certificate

Equipment :	SOUND CALIBRATOR
Manufacturer :	RION
Model :	NC-75
Serial No.:	35024431
ID No.:	BKK FS1221
Condition As Found :	GOOD
Customer :	ALS LABORATORY GROUP (THAILAND) CO., LTD. 104 PHATTHANAKAN 40, PHATTHANAKAN ROAD, KHWAENG PHATTHANAKAN, KHET SUAN LUANG, BANGKOK, 10250 THAILAND.

Location :	-	
Ambient Temperature :	(23.0 ± 3)	°C
Pressure :	(101.3 ± 3)	kPa
Relative Humidity :	(50.0 ± 20)	%

REVIEW BY ..... Nanakorn P.
APPROVED BY.....
NEXT CAL DATE.....10/01/26.....

Received Date :	23 DECEMBER 2024
Calibration Date :	10 JANUARY 2025
Date of Issue :	13 JANUARY 2025

Calibrated by : Nathakorn Pisutpaisan

Approved by : T. Petchurai
(Thanakul Petchurai)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

Cert. No. : ACC25002
Job No. : VC68AC0054
Pages : 2 of 3

Calibration Procedure : CP-AC-03

Calibration Method :

This equipment was calibrated by follow on IEC-60942-2003 Standard.
The sound pressure level, frequency and total distortion of the sound calibrator was measured using the reference microphone.

Condition of this result of calibration ;

1. Reference Standard Instruments :

Instrument	Model	Serial No.	Cert. No.	Due Date
Waveform Generator	33511B	MY52302742	EF-0007-24	05-FEB-25
Digital Multimeter	33461A	MY53220104	EEL.BP 21/0267	13-FEB-25
Digital Multimeter	33461A	MY53220076	EEL.BP 20/0267	15-FEB-25
Digital Multimeter	33461A	MY60024273	EEL.BP 22/0267	15-FEB-25
Programmable Attenuator	MAT-1070	62100114	EF-0008-24	05-FEB-25
Condenser Microphone	4180	2977900	AA-1001-24	12-FEB-25
Measuring Amplifier	NA-42KAI	34550495	AA-3001-24	05-FEB-25
Audio Analyzer	AVR-3360A	V744B6069	EF-0009-24	09-FEB-25

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.
3. This certificate is traceable to the international system of unit maintained at :
   3.1 National Institute of Metrology (Thailand).
   3.2 Thailand Institute of Scientific and Technological Research (TISTR).

SITHIPORN associates

SITHIPORN ASSOCIATES
CALIBRATION LABORATORY

Cert. No. : ACC25002
Job No. : VC68AC0054
Pages : 3 of 3

Result of calibration :

1. Sound pressure level

Specified sound pressure level (dB)	Measured value (dB)	Deviated value (dB)	Uncertainty (dB)	Acceptance limit (dB)
94	93.97	-0.03	0.14	0.40

2. Frequency

Specified Frequency (Hz)	Measured value (Hz)	Deviated value (%)	Uncertainty (%)	Acceptance limit (%)
1000	1000.0	0.0	0.1	1.0

3. Total distortion

Measured value (%)	Uncertainty (%)	Acceptance limit (%)
0.37	0.10	3.0

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor $k = 2$ or any value following calculation,providing a lavel of confidence of approximately 95 %

End of Calibration Certificate

SITHIPORN ASSOCIATES CO., LTD.
CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplad, Bangkok, 10700 Thailand
Tel. +66 2433 8331 Email : calibration@sithiphorn.com

Cert. No. : ACL24262
Pages : 1 of 8

Calibration Certificate

Equipment :	SOUND LEVEL METER
Manufacturer :	RION
Model :	NL-42 / Microphone UC-52 / Preamplifier NH-24
Serial No.:	00658242 / 157782 / 48097
ID No.:	BKK_FS0099

Condition As Found : GOOD

Customer : ALS LABORATORY GROUP (THAILAND) CO., LTD.
104 PHATTHANAKAN 40, PHATTHANAKAN ROAD,
KHWAENG PHATTHANAKAN, KHET SUAN LUANG,
BANGKOK, 10250 THAILAND.

Location :	-	
Ambient Temperature :	(23.0 ± 3)	°C
Pressure :	(101.3 ± 3)	kPa
Relative Humidity :	(50.0 ± 20)	%

REVIEW BY Nuchsom P.
APPROVED BY
NEXT CAL. DATE 30/8/25

Received Date : 09 AUGUST 2024
Calibration Date : 30 AUGUST 2024
Date of Issue : 03 SEPTEMBER 2024

Calibrated by : Nathakorn Pisutpaisan

Approved by : T. Petchurai
(Thanakul Petchurai)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

SITHIPORN ASSOCIATES CO., LTD.
CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplad, Bangkok, 10700 Thailand
Tel. +66 2433 8331 Email : calibration@sithiphorn.com

Cert. No. : ACL24262
Job No. : VC67AC0139
Pages : 2 of 8

Calibration Procedure : CP-AC-01

Calibration Method :

This equipment was calibrated by follow on IEC-61672-3 (2013) Standard for sound level meter (SLM).
The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.
For tests results of each items were made by observation of each Instruments display and also with SLM's display.

Condition of this result of calibration :

1. Reference Standard Instruments :

Instrument	Model	Serial No.	Cert. No.	Due Date
Waveform Generator	33210A	MY48017076	EF-0009-24	05-FEB-25
Waveform Generator	33511B	MY52302742	EF-0007-24	05-FEB-25
Digital Multimeter	34461A	MY53220104	EEL.BP 21/0267	13-FEB-25
Digital Multimeter	34461A	MY53220076	EEL.BP 20/0267	15-FEB-25
Digital Multimeter	34461A	MY60024273	EEL.BP 22/0267	15-FEB-25
Programmable Attenuator	MAT-1070	62100114	EF-0008-24	05-FEB-25
Condenser Microphone	4180	2977900	AA-1001-24	12-FEB-25
Measuring Amplifier	NA-42KAI	34560495	AA-3001-24	05-FEB-25

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.
3. This certificate is traceable to the international system of unit maintained at :
   3.1 National Institute of Metrology (Thailand).
   3.2 Thailand Institute of Scientific and Technological Research (TISTR).

T. Petchurai.

SITHIPORN ASSOCIATES CO., LTD.
CALIBRATION LABORATORY
451-461/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok 10700 Thailand
Tel. +66 2433 8331 Email : calibration@sithiphorn.com

SITHIPORN associates

NSC-TISI-TIS 17025
CALIBRATION 0394

Cert. No. : ACL24262
Job No. : VC67AC0139
Pages : 3 of 8

Summary of Measurement Result :

Parameter	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	0.2	N/A
2. Self-generated noise	0.2	N/A
3. Acoustical signal tests of frequency weightings		
125 Hz	0.3	0.6
1000 Hz	0.3	0.6
8000 Hz	0.3	0.7
4. Electrical signal tests of frequency weightings		
For 10 Hz to 4 kHz	0.3	0.6
For >4 kHz to 10 kHz	0.3	0.7
For > 10 kHz to 20 kHz	0.3	1.0
5. Frequency and time weightings at 1 kHz	0.2	0.2
6. Long - term stability	0.1	0.1
7. Level linearity on the reference level range	0.2	0.3
8. Level linearity including the level range control	0.2	0.3
9. Tone burst response	0.2	0.3
10. Peak C sound level	0.2	0.35
11. Overload indication	0.2	0.25
12. High level stability	0.1	0.1

SITHIPORN ASSOCIATES CO., LTD.
CALIBRATION LABORATORY
451-461/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok 10700 Thailand
Tel. +66 2433 8331 Email : calibration@sithiphorn.com

SITHIPORN associates

NSC-TISI-TIS 17025
CALIBRATION 0394

Cert. No. : ACL24262
Job No. : VC67AC0139
Page : 4 of 8

Result of calibration :

1. Absolute sensitivity

Reference Acoustic Signal (dB)	Measured Value (dB)	Deviation (dB)	Acceptance Limit (dB)
93.9 (93.94)	93.9	0.0	±0.3

2. Self-generated noise

2.1 Normal test

Measured Value (dB)
17.4

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Weighting (dB)
A - weight	15.4
C - weight	21.4
Flat	27.2

3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
125	0.1	0.2	0.2	± 1.5
1000	-0.1	-0.1	-0.1	± 1.0
8000	-1.5	-1.5	-1.4	±5.0

SITHIPORN ASSOCIATES CO., LTD.
CALIBRATION LABORATORY
451-461 Sirinthorn Road. Bangbumru, Bangplud, Bangkok, 10700 Thailand
Tel. +66 2433 8331 Email : calibration@sithiphorn.com

4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	-0.1	0.0	0.0	±2.0
125	0.0	0.0	0.0	±1.5
250	0.0	0.0	0.0	±1.5
500	0.0	0.0	0.0	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.0	0.0	±2.0
4000	0.0	0.0	0.0	±3.0
8000	0.0	0.1	0.1	±5.0

5. Frequency and time weightings at 1 kHz

5.1 Frequency weightings at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.2
C - weight	94.0	94.0	0.0	± 0.2
Flat	94.0	94.0	0.0	± 0.2

5.2 Time weighting at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	94.0	94.0	0.0	± 0.1
Slow	94.0	94.0	0.0	± 0.1
Leq	94.0	94.0	0.0	± 0.1

6. Long - term stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.3

T. Rotchn.

SITHIPORN ASSOCIATES CO., LTD.
CALIBRATION LABORATORY
451-461 Sirinthorn Road. Bangbumru, Bangplud, Bangkok, 10700 Thailand
Tel. +66 2433 8331 Email : calibration@sithiphorn.com

7. Level linearity on the reference level range

Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
137.0	137.0	0.0	± 1.1
136.0	136.0	0.0	± 1.1
135.0	135.0	0.0	± 1.1
134.0	134.0	0.0	± 1.1
133.0	133.0	0.0	± 1.1
132.0	132.0	0.0	± 1.1
131.0	131.0	0.0	± 1.1
129.0	129.0	0.0	± 1.1
124.0	124.0	0.0	± 1.1
119.0	119.0	0.0	± 1.1
114.0	114.0	0.0	± 1.1
109.0	109.0	0.0	± 1.1
104.0	104.0	0.0	± 1.1
99.0	99.0	0.0	± 1.1
94.0	94.0	0.0	± 1.1
89.0	89.1	0.1	± 1.1
84.0	84.1	0.1	± 1.1
79.0	79.0	0.0	± 1.1
74.0	74.1	0.1	± 1.1
69.0	69.1	0.1	± 1.1
64.0	64.0	0.0	± 1.1
59.0	59.1	0.1	± 1.1
54.0	54.0	0.0	± 1.1
49.0	49.0	0.0	± 1.1
44.0	44.0	0.0	± 1.1
39.0	39.0	0.0	± 1.1
34.0	34.1	0.1	± 1.1
30.0	30.2	0.2	± 1.1
29.0	29.3	0.3	± 1.1
28.0	28.4	0.4	± 1.1
27.0	27.5	0.5	± 1.1
26.0	26.6	0.6	± 1.1
25.0	25.7	0.7	± 1.1

T. Rotchn.

SITHIPORN ASSOCIATES CO., LTD.
CALIBRATION LABORATORY
451-451/1 Sirinthorn Road, Bangsumru, Bangplud, Bangkok, 10700 Thailand
Tel. +66 2433 8331 Email : calibration@sithiphorn.com

NSC-TISI-TIS 17025 CALIBRATION 0394

Cert. No. : ACL24262
Job No. : VC67AC0139
Pages : 7 of 8

8. Level linearity including the level range control

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
130	94.0	94.0	0.0	±1.1

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
130	30.0	30.1	0.1	±1.1

9. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Cycle	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.0	0.0	±1.0
Slow	2	8	108.0	108.0	0.0	1.5 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
SEL	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.0	0.0	±1.0

T. Petch.

SITHIPORN ASSOCIATES CO., LTD.
CALIBRATION LABORATORY
451-451/1 Sirinthorn Road, Bangsumru, Bangplud, Bangkok, 10700 Thailand
Tel. +66 2433 8331 Email : calibration@sithiphorn.com

NSC-TISI-TIS 17025 CALIBRATION 0394

Cert. No. : ACL24262
Job No. : VC67AC0139
Pages : 8 of 8

10. Peak C sound level

Number of cycle in test signal	Anticipated Value (dB)	Measured Value, Lcpeak (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	±3.0
One	136.4	136.3	-0.1	±3.0

Number of cycle in test signal	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	±2.0
Positive half cycle	135.4	135.2	-0.2	±2.0
Negative half cycle	135.4	135.2	-0.2	±2.0

11. Overload indication

Measured value (dB)		Deviated Value (dB)	Acceptance Limits (dB)
Positive one-half cycle	Negative one-half cycle		
89.8	89.5	-0.3	±1.5

12. High level stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor $k = 2$ or any value following calculation,providing a lavel of confidence of approximately 95 %

End of Calibration Certificate

T. Petch.

SCG
Metrology
SCI ECO Services Company Limited
33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110, Thailand.
Saraburi Tel : +66 3627 3096 Fax : +66 3627 3100
Bangkok Tel : +668 9205 6851 , +669 8247 2360
Website : www.scieco.co.th E-Mail : calibrate@scg.com

NSC-TISI-TIS 17025
CALIBRATION 0244

Certificate of Calibration

Equipment	:	Chamber (Cooling Room)
Manufacturer	:	KOLDTECH
Model	:	KM 320
Serial No.	:	TBN-1012061/05
Customer Code	:	BKK_EN0167
ID No.	:	T2463A3
Customer	:	ALS Laboratory Group (Thailand) Co.,Ltd.
		104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan,
		Khet Suan Luang, Bangkok 10250
Customer Location	:	Laboratory
Date of Receipt	:	29 November 2023
Calibrated By	:	Atiphong Rongrat (Technician)
Approved By	:	/ Boonchai Suriyawong (Site Calibration Manager)
Date of Issue	:	09 JAN 2024

REVIEW BY Kanlaya A.
APPROVED BY Sirilak P.
NEXT CAL. DATE 06/06/25

The uncertainties are for a confidence probability of approximately 95%.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standard laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Metrology.

SCG
Metrology
SCI ECO Services Company Limited
33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110, Thailand.

NSC-TISI-TIS 17025
CALIBRATION 0244

Calibration Report

Equipment	:	**Chamber (Cooling Room)**
Date of Calibration	:	**6 December 2023**
Environment	:	**Temperature : 23.4-24.9 °C**
		Line Voltage : 221.4-230.2 V
		Relative Humidity : 55 - 65 %RH

Condition of this results of calibration :

1. Thisequipment was calibrated by insert 16 standard thermocouples type T into its chamber , the other one standard thermocouples type T use for ambient temperature measurement . The calibration was done in according to WI-T20 (based on ASTM E145-94 (Reapproved 2001) and AS2853-1986).
   All data show below were final values and the initial data from customer request . The temperature scale used was based on ITS - 90 .
2. Reference Standard Instrument :


Instrument	Model	Instrument No.	Certificate No.	Due Date
TC	TYPE T	TN161-TN170	T230773	10 April 2024
TC	TYPE T	TN171-TN180	T230773	10 April 2024
DATA LOGGER	34970A	T149	T230773	10 April 2024

3. This certificate is traceable to :
   National Institute of Metrology (Thailand) through Metrological Center (NSC-TISI-TIS 17025 CALIBRATION 0244)
4. Condition of calibrated item : good
   Equipment Description :
   Time Constant 1 Hour 30 Minute At 3 °C
   Fresh Air Damper ☐ Open ☐ Min ☐ Medium ☐ Max
   ☐ Close
   ☒ Not Available
5. Adjustment :
   (X) without adjustment ( ) after adjustment

Approved By.

Certificate No. T232160

Calibration Report

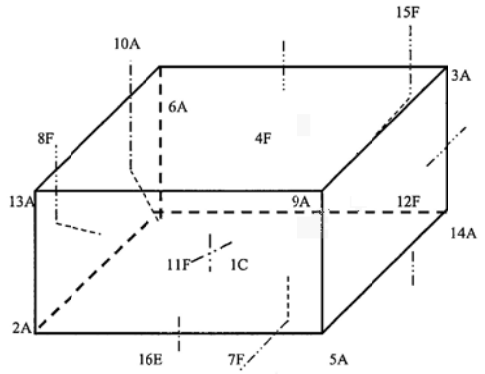

C = Centre , F = Centre of Face , A = Corner , E = Centre of Edge

1C	= TN161	12F	= TN172
2A	= TN162	13A	= TN173
3A	= TN163	14A	= TN174
4F	= TN164	15F	= TN175
5A	= TN165	16E	= TN176
6A	= TN166		
7F	= TN167		
8F	= TN168		
9A	= TN169		
10A	= TN170		
11F	= TN171		

Approved By.

SCG Metrology
SCI ECO Services Company Limited
33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110, Thailand.
NSC-TISI-TIS 17025
CALIBRATION 0244

Certificate No. T232160

Calibration Report

Measurement Results

	Average Standard Reading at each position (°C)											
Calibration Point	TN161	TN162	TN163	TN164	TN165	TN166	TN167	TN168	TN169	TN170	TN171	TN172
3.0	2.83	3.34	2.95	3.46	3.45	3.76	3.25	3.46	3.39	3.50	3.58	3.42
	TN173	TN174	TN175	TN176								
	3.33	3.39	3.15	3.43								

Chamber (Cooling Room)			Temperature Distribution				
Setting (°C)	Reading (°C)		Average (°C)	Stability (±°C)	Uniformity (°C)	Uncertainty (±°C)	Coverage Factor *k*
	Min , Max	Average					
3.0	2.8 , 4.1	3.5	3.36	1.10	2.00	1.90	2.09

The calibration result apply only the above calibrated item.
The result of test was found accurate as shown on date and place of test only.
The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor *k* which for a t-distribution, providing a level of confidence of approximately 95 % .

Approved By.

SCG

Metrology Center
SCI ECO Services Company Limited
51 Moo 8, Tubkwang, Kaeng Khoi, Saraburi, Thailand 18260
Bangkok Tel : +668 9205 6851 , +669 81924 0059
Saraburi Tel : +669 8247 2360
Website : www.scieco.co.th E-Mail : calibrate@scg.co.th

NSC-TISI-TIS 17025
CALIBRATION 0244

Certificate No. T250873

Page 1 of 4

Certificate of Calibration

Equipment	:	Chamber (Cooling Room)
Manufacturer	:	KOLDTECH
Model	:	KM 320
Serial No.	:	TBN-1012061/05
Customer Code	:	BKK_EN0167
ID No.	:	T2463A3
Customer	:	ALS Laboratory Group (Thailand) Co.,Ltd. 104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan, Khet Suan Luang, Bangkok 10250
Customer Location	:	Laboratory Room
Date of Receipt	:	28 May 2025
Calibrated By	:	Atiphong Rongrat (Technician)
Approved By	:	/ Boonchai Suriyawong (Site Calibration Manager)
Date of Issue	:	19 JUN 2025

REVIEW BY ..... Sirilak K.....

APPROVED BY ..... Sirilak P.....

NEXT CAL DATE..... 04/12/26 .....

The uncertainties are for a confidence probability of approximately 95%.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standard laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Metrological Center.

SCG

Metrology Center
SCI ECO Services Company Limited
51 Moo 8, Tubkwang, Kaeng Khoi, Saraburi, Thailand 18260

NSC-TISI-TIS 17025
CALIBRATION 0244

Calibration Report

Equipment	:	**Chamber (Cooling Room)**
Date of Calibration	:	**4 June 2025**
Environment	:	**Temperature : 23.4-24.9 °C**
		Line Voltage : 221.4-230.2 V
		Relative Humidity : 55 - 65 %RH

Condition of this results of calibration :

1. Thisequipment was calibrated by insert 16 standa'd thermocouples type T into its chamber , the other ore standard thermocouples type T use for ambient temperature measurement . The calibration was done in according to WI-T20 (based on ASTM E145-94 (Reapproved 2001) and AS2853-1986).
   All data show below were final values and the initial data from customer request . The temperature scale used was based on ITS - 90 .
2. Reference Standard Instrument :


Instrument	Model	Instrument No.	Certificate No.	Due Date
TC	TYPE T	TN91-TN100	T242036	3 December 2025
TC	TYPE T	TN101-TN110	T242036	3 December 2025
DATA LOGGER	34970A	T121	T242036	3 December 2025

3. This certificate is traceable to :
   National Institute of Metrology (Thailand) through Metrological Center (NSC-TISI-TIS 17025 CALIBRATION 0244.)
4. Condition of calibrated item : good
   Equipment Description :
   Time Constant 2 Hour 20 Minute At 3 °C
   Fresh Air Damper ☐ Open ☐ Min ☐ Medium ☐ Max
   ☐ Close
   ☒ Not Available
5. Adjustment :
   (X) without adjustment ( ) after adjustment

Approved By. _____

Certificate No. T250873

Calibration Report

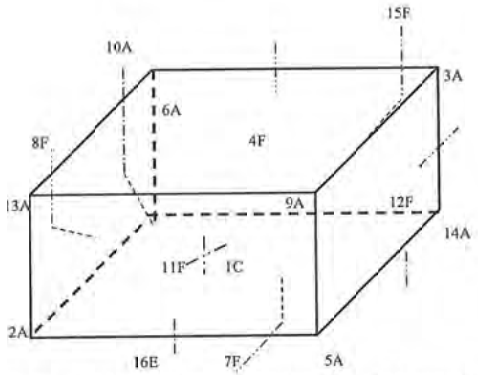

C = Centre , F = Centre of Face , A = Corner , E = Centre of Edge

1C	= TN91	
2A	= TN92	
3A	= TN93	
4F	= TN94	
5A	= TN95	
6A	= TN96	
7F	= TN97	
8F	= TN98	
9A	= TN99	
10A	= TN100	
11F	= TN101	

12F	= TN102
13A	= TN103
14A	= TN104
15F	= TN105
16E	= TN106

Approved By. _____

SCG
Metrology Center
SCI ECO Services Company Limited
51 Moo 8, Tubkwang, Kaeng Khoi, Saraburi, Thailand 18260
NSC-TISI-TIS 17025 CALIBRATION 0244

Certificate No. T250873

Calibration Report

Measurement Results

Calibration Point	Average Standard Reading at each position (°C)											
	TN91	TN92	TN93	TN94	TN95	TN96	TN97	TN98	TN99	TN100	TN101	TN102
3.0	2.95	2.92	3.05	2.92	3.16	3.50	3.40	3.03	3.14	2.98	3.44	3.13
	TN103	TN104	TN105	TN106								
	3.19	3.06	3.46	2.92								

Chamber (Cooling Room)			Temperature Distribution				
Setting (°C)	Reading (°C)		Average (°C)	Stability (±°C)	Uniformity (°C)	Uncertainty (±°C)	Coverage Factor *k*
	Min , Max	Average					
3.0	2.8 , 3.9	3.4	3.14	1.20	1.30	1.90	2.04

The calibration result apply only the above calibrated item.
The result of test was found accurate as shown on date and place of test only.
The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor *k* which for a t-distribution, providing a level of confidence of approximately 95 % .

Approved By. _____

TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL.0-2717-3000-29 FAX.0-2719-9484

NSC-TISI-TIS17025
CALIBRATION 0008

Certificate of Calibration

Cert.No.: 24CG952
Page.: 1 of 2

Equipment :	Burette
Capacity :	50 mL
Serial No. :	-
ID. No. :	BKK_EN0171
Manufacturer :	Witeg
Made in :	Germany

REVIEW BY Siriluk P.
APPROVED BY
NEXT CAL DATE 27/08/25

Submitted by : ALS Laboratory Group (Thailand) Co.,Ltd.
104 Phatthanakan 40, Phatthanakan Rd.,
Khwaeng Phatthanakan, Khet Suan Luang,
Bangkok 10250 Thailand

Ambient Temperature :	(20 ± 2.5) °C
Relative Humidity :	(50 ± 10) %
Barometric Pressure :	760 mmHg
Calibration Procedure :	ASTM E 542 - 01
Calibrated by :	Natcha Chayyingcheiw

Approved by :

Approved Signatory

( ) Unnopphol Harachai
(✓) Srisuda Khamtha
( ) Sa-ngeunkam Wongsa

Issue Date : 27 February 2024

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

Equipment :	Burette
Received Date :	23 February 2024
Condition As-Received :	New Item
Calibration Date :	27 February 2024
Reference :	2402-0757DSC-1

Condition of this result of calibration

1. Reference Standard Instruments :

Instruments	Model	Serial No.	ID. No.	Certificate No.	Traceability	Due date
1) Balance	XP205DR	1126143764	140RC004	23MM538	TPA	15 Sep 2024
2) Thermo-Hygrograph	THDX-CE	00016540	140EC001	23H1275	TPA	09 June 2024
3) Thermometer	-	0834181	140EC005	23I948	TPA	10 Aug 2024

This certification is traceable to SI Unit

2. The certificate is valid only to the item calibrated on date and place of calibration.
3. True value is converted to true volume at the standard temperature of 20 °C

Calibration result :

Nominal capacity (mL)	Reading (mL)	Uncertainty (± mL)	*k* Factor
50	50.0032	0.010	2.00

Remark mL = cm^3

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k* , providing a level of confidence of approximately 95 %.

-o0o-

TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL.0-2717-3000-29 FAX.0-2719-9484

ilac-MRA

NSC-TISI-TIS17025
CALIBRATION 0008

Certificate of Calibration

Cert.No.: 24CH1295
Page.: 1 of 3

Equipment :	pH Meter
Manufacturer :	Hach
Model :	HQ411d
Serial No. :	200100031163
ID No. :	BKK_EN0342
Condition As-Received:	Used Item
Received Date :	16 October 2024
Calibration Date :	17 October 2024
Reference :	2410-0548DSC-5
Submitted by :	ALS Laboratory Group (Thailand) Co.,Ltd. 104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan, Khet Suan Luang, Bangkok 10250 Thailand
Ambient Temperature :	(25 ± 2.5) °C
Relative Humidity :	(50 ± 15) %
Calibration Procedure :	In - house method : - CP-CH5 by direct measurement with certified reference material (CRM) - CP-CH8 by comparison with temperature standard
Calibrated by :	Warakorn Lerngagtrakul
Approved by :	Approved Signatory

REVIEW BY ..... linda K .....

APPROVED BY ..... Siriluk P .....

NEXT CAL DATE ..... 17/10/25 .....

( ) Unnopphol Harachai
( ) Ponpan Paipim
(✓) Saithip Meangmai

Issue Date : 21 October 2024

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

Condition of this calibration result

1. Reference Standard Instrument

Instrument	Serial No.	ID No.	Cert. No.	Due Date
1)Ref. Standard Thermometer	2188080	130RC044	2411022	16 Sep 2025

- This Certification is traceable to SI Throught Technology Promotion Association (Thailand - Japan)

2. Certified Reference Materials :The measurement results are traceable to SI through Hach Lenge GmbH Ltd. Deutsche Akkreditierungsstelle, Accredited No.D-RM-15184-01-00
:The measurement results are traceable to SI through CPA chem Ltd., ANSI-ASQ National Accreditation Board, Accredited No. AR-1835

Buffer Solution	Manufacturer	Lot No.	Exp. date
pH 4.008	CPA chem	1034203	27 Sep 2026
pH 6.999	Hach Lenge GmbH	C03145	28 Feb 2026
pH 10.010	CPA chem	1034205	27 Sep 2025

3. This certificate is valid only to the item calibrated on date and place of calibration.

Calibration Results

Function : pH Measurement

Performing three buffers standard curve by using buffer nominal pH (4,7,10)

Unit Under Calibration	Standard pH Buffer Solution	Actual pH Reading	Actual mV Reading (mV)	Uncertainty of pH Measurement (±)	Coverage factor *k*
pH Electrode	4.008	4.028	174.6	0.0044	2.00
S/N.: 230473042902	6.999	7.014	1.4	0.0084	2.05
	10.010	10.018	-172.8	0.0066	2.00

Remark - Can not connect the BNC because the plug does not match with the socket.

Cert.No.: 24CH1295
Page.: 3 of 3

Calibration Results

Function : Temperature Measurement

(*) Without adjustment

This equipment was connected with Temperature Probe;

- Model : PHC281
- Serial No. : 230473042902

Dimension of probe

- Length : 103 mm.
- Diameter : 12 mm.
- Immersion Depth : 90 mm.

Calibration Point (°C)	Standard Temperature (°C)	UUC* Reading (°C)	Error (°C)	Uncertainty of measurement (± °C)	Coverage factor *k*
25.0	25.002	25.0	-0.002	0.13	2.00

Remark : UUC* = Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

ID No. : BKK_EN0003

Manufacturer : Sartorius

Page No. : 1 Of 2

Customer Name : ALS Laboratory Group (Thailand)Co., Ltd.

104 Phatthanakan 40,Phatthanakan Rd., Khwaeng Suan Luang, Khet Suan Luang, Bangkok 10250.

Calibrated Place : Lab Room

Calibrated By : Mr.Chonchai Inthana

Calibration Date : Friday, August 02, 2024

Calibration Procedure No. : This calibration was conducted by Using in-house calibration procedure number (WI-003) Based on UKAS LAB 14 : 2019

Metrological data :

Capacity : 220 g Readability : 0.0001 g

Ambients Conditions:

Temperature : 23.0 °C ± 5.0 °C

Humidity : 55.0 % RH ± 10.0 % RH

Pressure : - ± -

Reasons for calibration

☐ New Installation ☐ Service / Repaired ☒ Re-calibration/ Maintenance

Equipment Condition: ☒ Good Operate ☐ Fair

Measurement Method UKAS Publication Ref :Lab 14

The measurement uncertainty stated is the expended uncertainty which is obtained from the standard uncertainty multiplied by the coverage factor (k=2) to provide a level of confidence of approximately 95%. It is determined in accordance with the Guide to Expression of Uncertainty in Measurement (GUM). The calibration certificate documents the traceability to National Standards, which realise the unit of measurement according to the International Standard System of Units (SI). Report of Tolerance came form list of Sartorius Metrological Specifications.

Traceability:

Model Number	Description	Traceability	Cetificate No.	Due Date
YCS011-522-00	Sartorius weight set 1mg - 5000g E2,YCS011-522-00	TCS	M23081975	23-Aug-2025
Testo 174 H	Thermo-Hygrometer , Testo 174H	ENTECH	H/T 661303,H661140	12-Nov-2024

This certificate relate and apply this equipment only.

This certificate may not be reproduced other than in full except with the prior written approval of the Verification Operation Division Sartorius (Thailand) Co., Ltd.

Mr.chonchai Inthana(Technical Manager)

STAMP

SARTORIUS ISO/IEC 17025:2017

SOP FM 33 03 February 2022

Sartorius (Thailand) Co., Ltd.
129 Rama 9 Road, Huaykwang, Huaykwang, Bangkok 10310
Tel +66 2643 8361-6 Fax +66 2643-8367, e-mail servicethailand@sartorius.com

SARTORIUS

Certificate of Calibration

Model Number :	MSE2245-100-DU	Certificate No. :	24BC0270
Description :	Analytical Balance	Issued Date :	Monday, August 05, 2024
Serial Number :	0027405555	Reference No. :	240912
ID No. :	BKK_EN0003		
Manufacturer :	Sartorius	Page No. :	2 of 2

Calibration Results : Without Adjustment

Repeatability


The reproducibility is the ability of a weighing instrument to display nearly identical readouts under constant test conditions when the same load within a measurement series is placed repeatedly on the weighing pan in the same manner. The standard deviation is used to express reproducibility quantitatively.

Nominal Value : (Low Load)	20.0000	200.0000
20 g	20.0000	199.9999
Tolerance	20.0001	200.0000
0.0001 g	20.0000	200.0000
	20.0000	200.0000
Nominal Value : (High Load)	20.0000	200.0000
200 g	20.0001	200.0001
Tolerance	20.0000	200.0000
0.0001 g	20.0000	199.9999
	20.0000	200.0000
Standard Deviation	0.00004	0.00006

Eccentricity (Off-center loading error)

The off-center loading error is yielded by the difference between the readout of the load, i.e. 1/3 or 1/4 of maximim capacity, placed in the middle of the weighing pan and between each of four additional measurement points (positions defined according to OIML R76).

Nominal value : 100 g
Tolerance 0.0004 g



	Difference
1	-
2	0.0000
3	0.0000
4	0.0000
5	0.0001
6	-

Linearity

The linearity, also called linearity error, Describes the deviation of the characteristic curve of a weighing instrument from the linear slope.

Tolerance 0.0002 g

Nominal Value (g)	Conventional Mass Value (g)	Displayed Value (g)	Deviation (g)	Uncertainty (g)
0.01	0.0100	0.0100	0.0000	0.00015
0.1	0.1000	0.1000	0.0000	0.00015
1	1.0000	1.0000	0.0000	0.00015
2	2.0000	2.0000	0.0000	0.00015
5	5.0000	5.0000	0.0000	0.00015
10	10.0000	10.0000	0.0000	0.00015
20	20.0000	20.0000	0.0000	0.00015
50	50.0000	50.0001	0.0001	0.00016
100	100.0000	100.0001	0.0001	0.00019
200	200.0000	200.0000	0.0000	0.00029

End of Report

REVIEW BY ..... Jinda K.

APPROVED BY ..... Sirilak P.

NEXT CAL DATE..... 29/10/25

Manufacturer :	Memmert
Model :	WNE29
Serial No. :	L622.0282
ID No. :	BKK_EN0439
Submitted by :	ALS Laboratory Group (Thailand) Co.,Ltd. 104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan, Khet Suan Luang, Bangkok 10250 Thailand
Location :	Organic Preparation Lab
Received Order :	29 October 2024
Calibration Date :	29 October 2024
Ambient Temperature :	(26 ± 10) °C
Relative Humidity :	(50 ± 30) %
Calibrated by :	Man Pattanapongpaiboon
Approved by :	Kunchit Approved Signatory

( ) Ponpan Paipim
( ) Suwit Imjai
(✓) Kunchit Promprat

Issue Date : 30 October 2024

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

Equipment : Water Bath
Condition As-Received : Used Item
Reference : 2410-0782OC-4

Cert. No.: 24TM1618
Page : 2 of 3

Procedure Used :-

Calibration were conducted using in-house calibration procedure CP-OT04 Based on ASTM E715 according to direct measurement method with Data Acquisition which connected with Industrial Platinum Resistance Thermometer (IPRT).

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-


Instrument	Serial No.	Cert. No.	Traceable	Due Date
1) Data Acquisition	MY57013711	24LM115	TPA	13 Jul 2025

2. This certificate is valid only to the item calibrated on date and place of calibration.
3. This certification is traceable to the International System of Unit.

Remark : TPA : Technology Promotion Association (Thailand - Japan)

Result of Calibration :- (*) Without Adjustment
Function of UUC* : Temperature Source
Heat transfer medium used : Water

	Environmental		AC Voltage Supply
	(°C)	(%R.H.)	(Volt)
Beginning of Calibration	25	54	222
Finished of Calibration	25	57	226

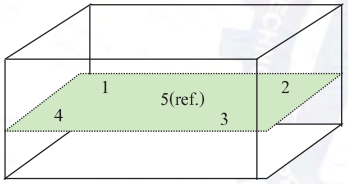

Front

Position :	Ref. Std. ID No.:
1	4803988-001
2	4803988-002
3	4803988-003
4	4803988-004
5(ref.)	4803988-005

Equipment : Water Bath
Condition As-Received : Used Item
Reference : 2410-0782OC-4
Result of Calibration :- (*) Without Adjustment
Function of UUC* : Temperature Source

Cert. No.: 24TM1618
Page : 3 of 3

Calibration point	UUC* Setting	UUC* Reading	Average* Standard Reading (°C) Position					Uncertainty
(°C)	(°C)	(°C)	1	2	3	4	5 (ref.)	(± °C)
85.0	85.0	85.0	85.133	85.212	85.150	84.983	85.096	0.22

Calibration point	Uniformity	Stability	Coverage Factor
(°C)	(°C)	(± °C)	*k*
85.0	0.21	0.13	2

Average* : The average of 30 values in each position.
Uniformity : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.
Stability : One-half of the greatest maximum difference of measured temperature at any one probe.
UUC* : Unit Under Calibration
Note : The reported uncertainty of measurement was included stability and excluded uniformity.

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor ***k***, providing a level of confidence of approximately 95 %.

-o0o-

Metrological Center
SCI ECO Services Company Limited
33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110
Telephone : +66 2 586 5792-4 Fax : +66 2 586 5109
Website : www.scieco.co.th E-Mail : calibrate@scg.co.th

Certificate of Calibration

Equipment	:	Digestion Unit
Manufacturer	:	SCP Science
Model	:	DigiPRER HT
Serial No.	:	HTC1120480658
Customer Code	:	BKK_EN0366
ID No.	:	T2635A5
Customer	:	ALS Laboratory Group (Thailand) Co.,Ltd.
		104 Phatthanakan 40, Phatthanakan Rd.,
		Khwaeng Phatthanakan, Khet Suan Luang, Bangkok 10250
Customer Location	:	Wet Chemistry Lab 1
Date of Receipt	:	2 April 2025
Calibrated By	:	Atiphong Rongrat (Technician)
Approved By	:	/ Boonchai Suriyawong (Site Calibration Manager)
Date of Issue	:	13 MAY 2025

REVIEW BY linda K
APPROVED BY Sirilak P
NEXT CAL. DATE 09/04/26

The uncertainties are for a confidence probability of approximately 95%.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standard laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Metrological Center.

Metrological Center
SCI ECO Services Company Limited
33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110
Telephone : +66 2 586 5792-4 Fax : +66 2 586 5109
Website : www.scieco.co.th E-Mail : calibrate@scg.co.th

Calibration Report

Equipment	:	**Digestion Unit**
Date of Calibration	:	9 April 2025
Environment	:	**Temperature : 23.9 - 26.3 °C**
		Line Voltage : 221.8 - 225.9 V
		Relative Humidity : 55 - 65 %RH

Condition of this results of calibration :

1. This equipment was calibrated by insert four standard thermocouples type S into its chamber , the other one thermocouple type T use for ambient temperature measurement . The calibration was done in according to WI-T10.
   All data show below were final values and the initial data from customer request . The temperature scale used was based on ITS - 90 .
2. Reference Standard Instrument :

Instrument	Model	Instrument No.	Certificate No.	Due Date
TC	Type S	M7-(CH1-CH4)	T242035	04 December 2025
DATA LOGGER	34970A	T121	T242035	04 December 2025

3. This certificate is traceable to :
   National Institute of Metrology (Thailand) through Metrological Center (NSC-TISI-TIS 17025 CALIBRATION 0244.)
4. Condition of calibrated item : good
   Equipment Description :
   Time Constant 2 Hour 40 Minute At 380 °C
   Fresh Air Damper ☐ Open ☐ Min ☐ Medium ☐ Max
   ☐ Close
   ☒ Not Available
5. Adjustment :
   (X) without adjustment ( ) after adjustment

Approved By. _____

Metrological Center


SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110

Telephone : +66 2 586 5792-4 Fax : +66 2 586 5109

Website : www.scieco.co.th E-Mail : calibrate@scg.co.th

Calibration Report

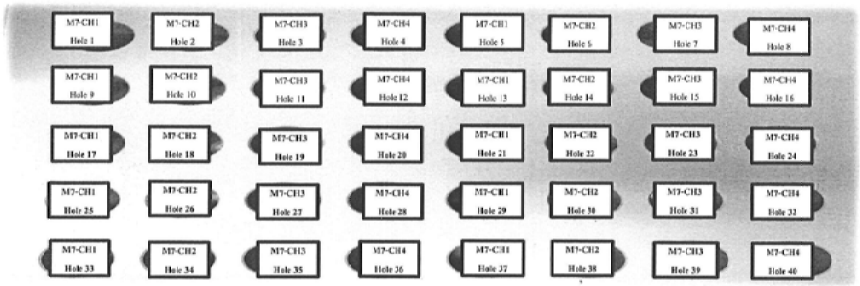

FRONT

Measurement Results

Cal. Point	Setting	Reading	STD.	Position of Stardards at Block							
(°C)	(°C)	(°C)	Reading	M7-CH1 Hole 1	M7-CH2 Hole 2	M7-CH3 Hole 3	M7-CH4 Hole 4	M7-CH1 Hole 5	M7-CH2 Hole 6	M7-CH3 Hole 7	M7-CH4 Hole 8
380.0	380.0	379.8 - 380.2	Max °C	380.0	381.0	380.9	379.6	380.3	380.9	381.3	380.1
			Min °C	379.6	380.8	380.6	379.3	379.9	380.5	380.5	379.6
			Average °C	**379.8**	**380.9**	**380.7**	**379.5**	**380.1**	**380.7**	**381.1**	**379.9**
			Stability ± °C	0.2	0.1	0.2	0.2	0.2	0.2	0.2	0.2

Cal. Point	Setting	Reading	STD.	Position of Stardards at Block							
(°C)	(°C)	(°C)	Reading	M7-CH1 Hole 9	M7-CH2 Hole 10	M7-CH3 Hole 11	M7-CH4 Hole 12	M7-CH1 Hole 13	M7-CH2 Hole 14	M7-CH3 Hole 15	M7-CH4 Hole 16
380.0	380.0	379.8 - 380.2	Max °C	378.9	378.7	379.8	381.0	382.8	381.3	381.7	380.4
			Min °C	378.3	378.2	379.3	380.7	382.1	380.5	381.3	380.0
			Average °C	**378.6**	**378.5**	**379.5**	**380.9**	**382.4**	**380.9**	**381.5**	**380.2**
			Stability ± °C	0.3	0.2	0.3	0.1	0.3	0.4	0.2	0.2

Approved By.

Metrological Center

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110

Telephone : +66 2 586 5792-4 Fax : +66 2 586 5109

Website : www.scieco.co.th E-Mail : calibrate@scg.co.th

Calibration Report

Measurement Results

Cal. Point	Setting	Reading	STD.	Position of Stardards at Block							
(°C)	(°C)	(°C)	Reading	M7-CH1 Hole 17	M7-CH2 Hole 18	M7-CH3 Hole 19	M7-CH4 Hole 20	M7-CH1 Hole 21	M7-CH2 Hole 22	M7-CH3 Hole 23	M7-CH4 Hole 24
380.0	380.0	379.8 - 380.2	Max °C	379.3	379.2	379.1	379.5	380.8	381.1	382.5	381.3
			Min °C	379.1	379.0	378.8	379.2	380.5	380.8	382.1	381.1
			Average °C	**379.2**	**379.1**	**379.0**	**379.3**	**380.6**	**380.9**	**382.3**	**381.2**
			Stability ± °C	0.1	0.1	0.1	0.1	0.2	0.2	0.2	0.1

Cal. Point	Setting	Reading	STD.	Position of Stardards at Block							
(°C)	(°C)	(°C)	Reading	M7-CH1 Hole 25	M7-CH2 Hole 26	M7-CH3 Hole 27	M7-CH4 Hole 28	M7-CH1 Hole 29	M7-CH2 Hole 30	M7-CH3 Hole 31	M7-CH4 Hole 32
380.0	380.0	379.8 - 380.2	Max °C	378.5	378.2	379.5	378.5	380.4	380.8	380.4	380.9
			Min °C	378.2	377.9	379.2	378.2	380.0	380.5	380.1	380.6
			Average °C	**378.3**	**378.0**	**379.4**	**378.3**	**380.2**	**380.7**	**380.2**	**380.8**
			Stability ± °C	0.2	0.2	0.1	0.2	0.2	0.1	0.2	0.2

Cal. Point	Setting	Reading	STD.	Position of Stardards at Block							
(°C)	(°C)	(°C)	Reading	M7-CH1 Hole 33	M7-CH2 Hole 34	M7-CH3 Hole 35	M7-CH4 Hole 36	M7-CH1 Hole 37	M7-CH2 Hole 38	M7-CH3 Hole 39	M7-CH4 Hole 40
380.0	380.0	379.8 - 380.2	Max °C	379.5	380.0	379.8	379.7	380.1	380.2	379.7	379.8
			Min °C	379.6	379.6	379.5	379.3	379.8	379.9	379.4	379.5
			Average °C	**379.8**	**379.8**	**379.7**	**379.5**	**379.9**	**380.1**	**379.5**	**379.7**
			Stability ± °C	0.2	0.2	0.1	0.2	0.2	0.2	0.2	0.1

The expanded uncertainty of temperature measurement was ±2.36 °C

The calibration result apply only the above calibrated item.

The result of test was found accurate as shown on date and place of test only.

The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor k=2 , providing a level of confidence of approximately 95 % .

Approved By.

บริษัท ดับเบิ้ล เอส ไดแอคนอสติคส์ จำกัด
DOUBLE S DIAGNOSTICS CO., LTD.
4 ซอยอุดมสุข 14 แขวงบางนา เขตบางนา กรุงเทพฯ 10260 โทรศัพท์: (02) 747-7009 โทรสาร: (02) 747-7008
4 Soi Udomsuk 14, Bangna, Bangkok 10260 Tel. (02) 747-7009 Fax: (02) 747-7008

Maintenance Plan YEAR : 2024

เดือน	Jan	Feb	Mar	Apr	May	Jun	Jul	Aug	Sep	Oct	Nov	Dec
ฉบ								✓				

Periodical maintenace check list for Konelab

	6M	12M	Note!
1.Diluent-wash tubing change	☐	☑	
2.ISE tubing change	☒	☒	none .
3.Syringe check/change		☑	
4.Dispensing check/ change		☑	
5.Waste tubing change when necessary		☑	
6.Lamp check/change	☐	☑	
7.Mixer paddle/paddle change(not Konelab20)		☑	
8.ISE needles check/change		☒	none .
9.Pump tubing check/ chance	☐	☑	
10.Broken/worn out part check /change		☑	
11.Peristaltic pump check /cleaning/ lubrication	☐	☑	
12.Heating check		☑	
13.Cooling check		☑	
14.Dispenser mechanic check/adjustment	☐	☑	
15.Cuvette transfer mechanic check/adjustment	☐	☑	
16.Dispenser movement check/adjustment	☐	☑	
17.Sample/reagent register check/adjustment	☐	☑	
18.Dispensing tubing tightness check	☐	☑	
19.Photometer and optics cleaning/check/adjustment	☐	☑	
20.Workstation PC cleaning if necessary	☐	☑	
21.Mechanic cleaning/lubrication	☐	☑	
22.Instrument cleaning if necessary	☐	☑	
23.Complete analyzer testing with waterblank/QC or sample	☐	☑	
24.Test parameters/Adjustment/config. Save to USB key	☐	☑	
25.UPS Test	☐	☑	

Place: ALS LAB **Instrument:** K30 Aquakem
Date/Time: 16/8/67 **Serial no:** 22781
Service done by: [signature] **Install date:** .....
Signature of customer: [signature] **Date/Time:** 16/08/2024

Accuracy results Aquakem 7.2.AQ2 Page: 1

Laboratory
Analyzer User

8/16/2024 14:53

Performed 8/16/2024
Lot WB34

ACCEPTANCE CRITERIA

	Result	Limit	Warning
Temperature (?C)	37.8	37.0 +/- 1.0	
Dispensing ratio	16.4	14.8 - 17.2	
CV%	0.29	<1.7	
Photometric noise			
Max SD L340_2 (mA)	0.17	<2.0	
Max SD L340_4 (mA)	0.87	<3.0	
Linearity of photometer			
Slope	1.0141	0.94 - 1.06	
Curvature	0.0053	+/- 0.02	
Max bias from linear fit (mA)	4.3	<15.0	
Max delta %	-1.6	+/- 6.0	
Linearity of sample dispensing			
Proport. volume XDISP2 (?l)	2.06	1.96 - 2.16	
Proport. volume XDISP4 (?l)	4.14	3.85 - 4.40	
XDISP2 CV%	1.21	<2.0	
XDISP4 CV%	0.90	<2.0	
XDISP10 CV%	0.68	<2.0	
Needle 0 ?l volume			
Average (A)	0.005	<0.050	
Standard deviation (A)	0.002	<0.005	
Volume (?l)	0.03	<0.32	

OTHER INFORMATION

Dispensing ratio

Posit	Result (A)
1	0.1549
2	0.1549
3	0.1537
4	0.1547
5	0.1547
6	0.1545

Photom. noise: SD (mA)

Posit	L340_2	L340_4
1	0.15	0.80
2	0.17	0.79
3	0.04	0.65
4	0.16	0.31
5	0.11	0.58
6	0.14	0.87

Laboratory
Analyzer User


8/16/2024 14:53

Linearity of sample dispensing

Test	Absorbance (A)
XDISP2	0.306
XDISP4	0.612
XDISP10	1.471

Linearity of photometer

L340	Target (A)	Meas (A)	Delta (A)	Delta %
1	0.002	0.006	-0.004	-217.7
2	0.486	0.493	-0.007	-1.5
3	1.451	1.469	-0.018	-1.2
4	1.936	1.963	-0.027	-1.4
5	2.415	2.454	-0.039	-1.6

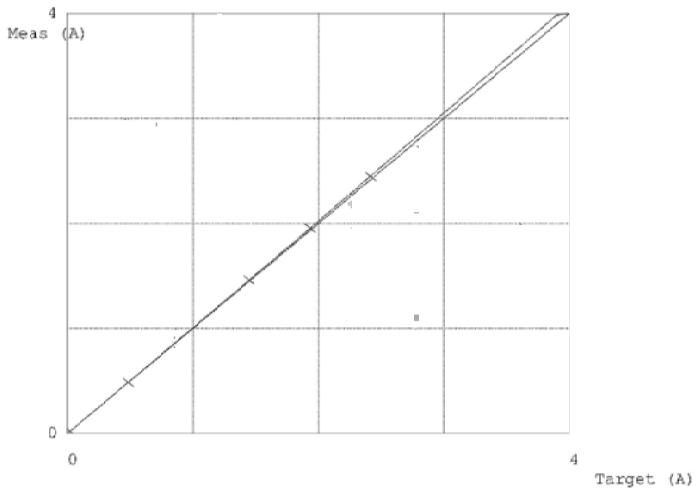

SCG

Metrology

SCI ECO Services Company Limited
33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110, Thailand.
Saraburi Tel : +66 3627 3096 Fax : +66 3627 3100
Bangkok Tel : +668 9205 6851 , +669 8247 2360
Website : www.scieco.co.th E-Mail : calibrate@scg.com

NSC-TISI-TIS 17025
CALIBRATION 0244

Certificate No. T240904 Page 1 of 3

Certificate of Calibration

Equipment : Chamber (Oven)

Manufacturer : Memmert

Model : UF 450

Serial No. : B717.0531

Customer Code : BKK_EN0273

ID No. : T8042A4

Customer : ALS Laboratory Group (Thailand) Co.,Ltd.
104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan,
Khet Suan Luang, Bangkok 10250

Customer Location : Laboratory (Oven Room)

Date of Receipt : 08 May 2024

Calibrated By : Preecha Phisassutthikul (Temperature Calibration Manager)

Approved By : _____ / Nuafun Sungchum (Metrology Manager)

Date of Issue : 23 MAY 2024

REVIEW BY Linda K.
APPROVED BY Siriluk P.
NEXT CAL. DATE 14/n/25

The uncertainties are for a confidence probability of approximately 95%.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standard laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Metrology.

Certificate No. T240904 Page 2 of 3

Calibration Report

Equipment : Chamber (Oven)
Date of Calibration : 14 May 2024
Environment : Temperature : 26.5-28.1 °C
Line Voltage : 226.7-229.8 V
Relative Humidity : 51 - 57 %RH

Condition of this results of calibration :

1. This equipment was calibrated by insert nine resistance thermometer detectors into its chamber , the other one resistance thermometer detector use for ambient temperature measurement . The calibration was done in according to WI-T20 (based on ASTM E145-94 (Reapproved 2001) and AS2853-1986).
All data show below were final values and the initial data from customer request . The temperature scale used was based on ITS - 90 .
2. Reference Standard Instrument :


Instrument	Model	Instrument No.	Certificate No.	Due Date
RTD	100 ohm	21-(CH1-10)	T231955	17 November 2024
DATA LOGGER	34970A	T121	T231955	17 November 2024

3. This certificate is traceable to :
National Institute of Metrology (Thailand) through Metrological Center (NSC-TISI-TIS 17025 CALIBRATION 0244.)
4. Condition of calibrated item : good
Equipment Description :
Time Constant 1 Hour 30 Minute At 104 °C
Fresh Air Damper ☐ Open ☐ Min ☐ Medium ☐ Max
☐ Close
☒ Not Available
5. Adjustment :
(X) without adjustment ( ) after adjustment

Approved By_____

Certificate No. T240904 Page 3 of 3

Calibration Report

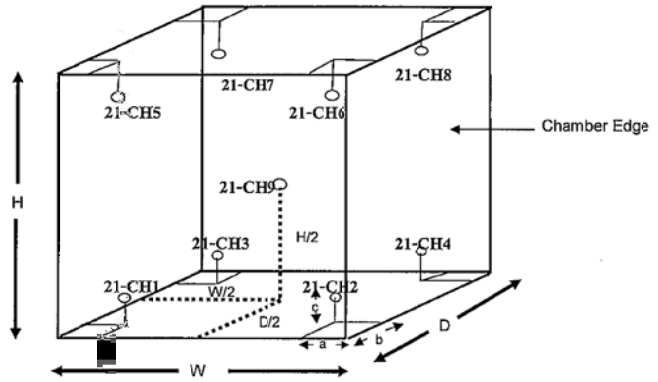

Remark :
Internal Dimensions of Chamber : W (Width) = 104 cm. , H(Height)=72 cm. and D(Depth)=60 cm.
Size of Installed Standard sensor number21-CH1 to number21-CH8 : a = 5 cm. ,b = 5 cm. and c = 5 cm.
Size of Installed Standard sensor number21-CH9 : W/2=104 cm./2 , H/2=72 cm./2 and D/2=60 cm./2

Measurement Results

	Average Standard Reading at each position (°C)								
Calibration Point	21-CH1	21-CH2	21-CH3	21-CH4	21-CH5	21-CH6	21-CH7	21-CH8	21-CH9
104	103.4	105.0	103.7	103.6	103.3	104.6	103.3	104.0	103.9
180	179.5	181.1	179.2	179.5	179.0	181.3	179.8	179.9	180.2

Chamber (Oven)			Temperature Distribution				
Setting (°C)	Reading (°C)		Average (°C)	Stability (±°C)	Uniformity (°C)	Uncertainty (±°C)	Coverage Factor *k*
	Min , Max	Average					
104.0	103.9 , 104	104.0	103.85	0.14	1.27	0.44	2.00
180.0	179.9 , 180.1	180.0	179.94	0.39	2.29	0.76	2.00

*** The quoted uncertainty exclude "uniformity"**
The calibration result apply only the above calibrated item.
The result of test was found accurate as shown on date and place of test only.
The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor *k* which for a t-distribution, providing a level of confidence of approximately 95 % .

End of Certificate

Approved By_____

TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3 : EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000 FAX. 0-2719-9484

Certificate of Testing

Equipment :	DO Meter
Manufacturer :	YSI
Model :	5000-230V
Serial No. :	09J101147
ID No. :	BKK_EN0017
Received Date :	15 November 2023
Test Date :	16 November 2023
Reference :	2311-0505DSC-4
Submitted by :	ALS Laboratory Group (Thailand) Co.,Ltd. 104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan, Khet Suan Luang, Bangkok 10250 Thailand
Laboratory Condition :	Temperature (25 ± 5) °C Humidity (50 ± 20) %
Test Procedure :	In - house method : CP-CH9 by Comparison Technique with Azide Modification Method
Tested by :	Walalak Sirithean
Approved by :	Approved Signatory

REVIEW BY Walak AL
APPROVED BY Siriluk P.
NEXT CAL. DATE 16/05/25

(√) Saithip Meangmai
( ) Warakorn Lerngagtrakul
( ) Ponpan Paipim

Issue Date : 17 November 2023

Condition of this result of calibration

1. Reference Standard Instruments :
   This certification is traceable to the Internaticnal System of Unit through the reference standards laboratory of Industrial Calibration Center, Technology Promotion Association (Thailand-Japan).

Instruments	Serial No.	ID No.	Certificate No.	Due Date
1) Burette	-	130BU10	23CG1172	22 Mar 2025
2) Balance	1124013382	140RC006	23MM18	20 Feb 2024

2. Standard Material :-

Material	Manufacturer	Lot.No.	Assay
Sodium Thiosulfate pentahydrate	Merck	AM1763316	100.2%

Result : **Dissolved Oxygen Meter Adjustment With Air 100 %**
Dissolved Oxygen Probe No.: 16K100498

Titration Method (Azide Modification Method) (mg/L)	DO Meter Reading (mg/L)	Standard Deviation (mg/L)
8.18	8.18	0.0055

This report was certified only for the instrument we tested.It is allowable to use for study the system efficiency,The environmental impact control and present to organization it may concerned Intend to use for advertising and referral purpose is prohibited.This report may not be reproduced other in full,without written approval of the laboratory

-o0o-

TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000-29 FAX. 0-2719-9484

NSC-TISI-TIS17025
CALIBRATION 0008

Cert. No.: 23LM192
Page.: 1 of 2

Certificate of Calibration

Equipment :	DO Meter with Sensor
Manufacturer :	YSI
Model :	5000-230V
Serial No. :	09J101147
ID No. :	BKK_EN0017
Submitted by :	ALS Laboratory Group (Thailand) Co.,Ltd. 104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan, Khet Suan Luang, Bangkok 10250 Thailand
Location :	TPA Chemistry Calibration Laboratory
Received Order :	15 November 2023
Calibrated Date :	16 November 2023
Ambient Temperature :	(26 ± 10) °C
Relative Humidity :	(50 ± 30) %
AC Line Voltage :	(220 ± 22) V
Calibrated by :	Kunchit Promprat
Approved by :	Approved Signatory

( ) Pornthippa Tameyakul
( ) Ponpan Paipim
(✓) Suwit Imjai

Issue Date : 17 November 2023

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

Equipment : DO Meter with Sensor
Condition As-Received : Used Item
Reference : 2311-0505DSC-10

Procedure Used :-

Calibration were conducted using in-house calibration procedure CP-DT01 according to comparison with Industrial Platinum Resistance Thermometer (IPRT) into Temperature Bath.

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

Instrument	Serial No.	Cert. No.	Traceable	Due Date
1) Digital Thermometer	3240076	23I305	TPA	15 Mar 2024

2. This certificate is valid only to the item calibrated on date and place of calibration.
3. This certification is traceable to the International System of Unit.

Remark : TPA : Technology Promotion Association (Thailand - Japan)

Result of Calibration :- (*) Without Adjustment

Function : Temperature measurement.

This instrument was connected with temperature sensor, S/N.: 16K100498

Calibration Point (°C)	Immersion Depth (mm)	Standard Temperature (°C)	UUC* Reading (°C)	Error (°C)	Uncertainty (± °C)	Coverage Factor *k*
20.0	60	19.997	19.93	-0.067	0.15	2.00

UUC* : Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor ***k***, providing a level of confidence of approximately 95 %.

-o0o-

TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3 : EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000 FAX. 0-2719-9484

Certificate of Testing

Cert.No.: 25TW101
Page.: 1 of 2

Equipment :	DO Meter
Manufacturer :	YSI
Model :	5000-230V
Serial No. :	09J101147
ID No. :	BKK_EN0017
Received Date :	19 May 2025
Test Date :	20 May 2025
Reference :	2505-0593DSC-1
Submitted by :	ALS Laboratory Group (Thailand) Co.,Ltd. 104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan, Khet Suan Luang, Bangkok 10250 Thailand
Laboratory Condition :	Temperature (25 ± 5) °C Humidity (50 ± 20) %
Test Procedure :	In - house method : CP-CH9 by Comparison Technique with Azide Modification Method
Tested by :	Walalak Sirithean
Approved by :	Approved Signatory

REVIEW BY ..... Sirilak P. .....
APPROVED BY ..... Sirilak P .....
NEXT CAL DATE..... 20/11/26 .....

( ) Chakrit Waewwanjua
( ) Ponpan Paipim
(✓) Saithip Meangmai

Issue Date : 20 May 2025

Cert.No.: 25TW101
Page.: 2 of 2

Condition of this result of calibration

1. Reference Standard Instruments :
   This measurement result is traceable to the International System of Unit through the reference standards laboratory of Industrial Calibration Center, Technology Promotion Association (Thailand-Japan).

Instruments	Serial No.	ID No.	Certificate No.	Due Date
1. Burette	-	130BU10	25CG1126	18 Mar 2027
2. Balance	14233821	110RC001	24MM131	04 July 2025

2. Standard Material :-

Material	Manufacturer	Lot.No.	Assay
Sodium Thiosulfate 5-Hydrate AR	KEMAUS	2203162447	99.6%

Result : **Dissolved Oxygen Meter Adjustment With Air 100 %**
Dissolved Oxygen Probe No.: 16K100498

Titration Method (Azide Modification Method) (mg/L)	DO Meter Reading (mg/L)	Standard Deviation (mg/L)
8.20	8.21	0.0090

This report was certified only for the instrument we tested.It is allowable to use for study Intend to use for advertising and referral purpose is prohibited.This report may not be reproduced other in full, without written approval of the laboratory

-o0o-

TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL.0-2717-3000-29 FAX.0-2719-9484

NSC-TISI-TIS17025
CALIBRATION 0008

Certificate of Calibration

Cert. No.: 25LM83
Page.: 1 of 2

Equipment :	DO Meter with Sensor
Manufacturer :	YSI
Model :	5000-230V
Serial No. :	09J101147
ID No. :	BKK_EN0017
Submitted by :	ALS Laboratory Group (Thailand) Co.,Ltd. 104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan, Khet Suan Luang, Bangkok 10250 Thailand
Location :	TPA On Site Calibration Laboratory
Received Order :	19 May 2025
Calibrated Date :	20 May 2025
Ambient Temperature :	(26 ± 10) °C
Relative Humidity :	(50 ± 30) %
AC Line Voltage :	(220 ± 22) V
Calibrated by :	Warakorn Lerngagtrakul
Approved by :	Kunchit Approved Signatory

( ) Chakrit Waewwanjua
( ) Suwit Imjai
(✓) Kunchit Promprat

Issue Date : 26 May 2025

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

Procedure Used :-

Calibration were conducted using in-house calibration procedure CP-OT01 according to comparison with Industrial Platinum Resistance Thermometer (IPRT) into Temperature Bath.

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

Instrument	Serial No.	Cert. No.	Traceable	Due Date
1) Digital Thermometer	2188080	24I1022	TPA	17 Sep 2025

2. This certificate is valid only to the item calibrated on date and place of calibration.
3. This certification is traceable to the International System of Unit.

Remark : TPA : Technology Promotion Association (Thailand - Japan)

Result of Calibration :- (*) Without Adjustment

Function : Temperature measurement.

This instrument was connected with temperature sensor, S/N.: 16K100498

Calibration Point (°C)	Immersion Depth (mm)	Standard Temperature (°C)	UUC* Reading (°C)	Error (°C)	Uncertainty (± °C)	Coverage Factor *k*
20.00	60	20.003	19.92	-0.083	0.15	2.00

UUC* : Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor ***k***, providing a level of confidence of approximately 95 %.

-o0o-

SCG

Metrology

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110, Thailand.

Saraburi Tel : +66 3627 3096 Fax : +66 3627 3100

Bangkok Tel : +668 9205 6851 , +669 8247 2360

Website : www.scieco.co.th E-Mail : calibrate@scg.com

NSC-TISI-TIS 17025 CALIBRATION 0244

Certificate No. T250356

Certificate of Calibration

Equipment	:	Chamber (Incubator)
Manufacturer	:	Memmert
Model	:	ICP 750
Serial No.	:	F819.0021
Customer Code	:	BKK_EN0304
ID No.	:	T9572A4
Customer	:	ALS Laboratory Group (Thailand) Co.,Ltd.
		104 Phatthanakan 40, Phatthanakan Rd.,
		Khwaeng Phatthanakan, Khet Suan Luang, Bangkok 10250
Customer Location	:	Wet Chemistry Lab 2
Date of Receipt	:	26 February 2025
Calibrated By	:	Atiphong Rongrat (Technician)
Approved By	:	_____ / Boonchai Suriyawong (Site Calibration Manager)
Date of Issue	:	17 MAR 2025

REVIEW BY Jinda K.
APPROVED BY Siriluk P.
NEXT CAL. DATE 04/03/26.

The uncertainties are for a confidence probability of approximately 95%.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standard laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Metrology.

SCG

Metrology

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110, Thailand.

NSC-TISI-TIS 17025 CALIBRATION 0244

Certificate No. T250356

Calibration Report

Equipment	:	**Chamber (Incubator)**
Date of Calibration	:	**4 March 2025**
Environment	:	**Temperature : 24.5-24.7 °C**
		Line Voltage : 221.4-224.7 V
		Relative Humidity : 55 - 65 %RH

Condition of this results of calibration :

1. This equipment was calibrated by insert 12 resistance thermometer detectors into its chamber , the other one resistance thermometer detector use for ambient temperature measurement . The calibration was done in according to WI-T20 (based on ASTM E145-94 (Reapproved 2019) and AS2853-1986),
   All data show below were final values and the initial data from customer request . The temperature scale used was based on ITS - 90 .
2. Reference Standard Instrument :


Instrument	Model	Instrument No.	Certificate No.	Due Date
RTD	100 ohm	31-(CH1-10)	T240399	16 March 2025
RTD	100 ohm	32-(CH1-10)	T240399	16 March 2025
DATA LOGGER	34970A	T193	T240399	16 March 2025

3. This certificate is traceable to :
   National Institute of Metrology (Thailand) through Metrological Center (NSC-TISI-TIS 17025 CALIBRATION 0244.)
4. Condition of calibrated item : good
   Equipment Description :
   Time Constant 2 Hour 10 Minute At 20 °C
   Fresh Air Damper ☐ Open ☐ Min ☐ Medium ☐ Max
   ☐ Close
   ☒ Not Available
5. Adjustment :
   (X) without adjustment ( ) after adjustment

Approved By: _____

Certificate No. T250356

Calibration Report

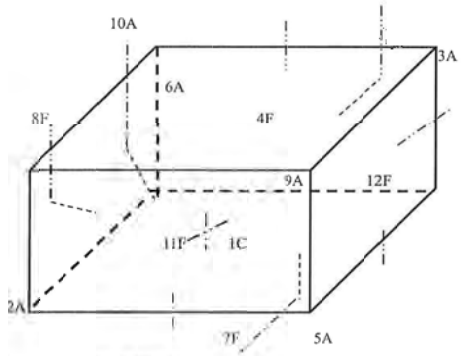

C = Centre , F = Centre of Face , A = Corner , E = Centre of Edge

1C	= 31-CH1
2A	= 31-CH2
3A	= 31-CH3
4F	= 31-CH4
5A	= 31-CH5
6A	= 31-CH6
7F	= 31-CH7
8F	= 31-CH8
9A	= 31-CH9
10A	= 31-CH10
11F	= 32-CH1
12F	= 32-CH2

Approved By.

SCG Metrology
SCI ECO Services Company Limited
33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110, Thailand.
NSC-TISI-TIS 17025
CALIBRATION 0244

Certificate No. T250356

Calibration Report

Measurement Results :

Calibration Point	Average Standard Reading at each position (°C)											
	31-CH1	31-CH2	31-CH3	31-CH4	31-CH5	31-CH6	31-CH7	31-CH8	31-CH9	31-CH10	32-CH1	32-CH2
20	20.02	20.42	19.96	20.23	19.83	19.44	19.71	20.01	20.06	20.04	20.13	19.98

Chamber (Incubator)			Temperature Distribution				
Setting (°C)	Reading (°C)		Average (°C)	Stability (±°C)	Uniformity (°C)	Uncertainty (±°C)	Coverage Factor *k*
	Min , Max	Average					
20.0	-	20.0	19.99	0.10	0.43	0.38	2.02

The calibration result apply only the above calibrated item.

The result of test was found accurate as shown on date and place of test only.

The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor *k* which for a t-distribution, providing a level of confidence of approximately 95 % .

End of Certificate

Approved By.

SCG

Metrology

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110, Thailand.

Saraburi Tel : +66 3627 3096 Fax : +66 3627 3100

Bangkok Tel : +668 9205 6851 , +669 8247 2360

Website : www.scieco.co.th E-Mail : calibrate@scg.com

NSC-TISI-TIS 17025
CALIBRATION 0244

Certificate No. T250353

Certificate of Calibration

Equipment : **Autoclave**

Manufacturer : **TOMY**

Model : **SX-700**

Serial No. : **48134190**

Customer Code : **BKK_ML0041**

ID No. : **T7725A3**

Customer : **ALS Laboratory Group (Thailand) Co.,Ltd.**

104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan,

Khet Suan Luang, Bangkok 10250

Customer Location : **Washing Room**

Date of Receipt : **26 February 2025**

Calibrated By : **Boonchai Suriyawong (Site Calibration Manager)**

Approved By : _____ **/ Sujjar Naknakred (Site Calibration Manager)**

Date of Issue : 10 MAR 2025

REVIEW BY .....

APPROVED BY .....

NEXT CAL. DATE 01/09/26

The uncertainties are for a confidence probability of approximately 95%.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standard laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Metrology.

SCG

Metrology

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110, Thailand.

NSC-TISI-TIS 17025
CALIBRATION 0244

Certificate No. T250353

Calibration Report

Equipment : **Autoclave**
Date of Calibration : **4 March 2025**
Environment : **Temperature : 22.2-25.4 °C**
Line Voltage : 221.1-224.7 V
Relative Humidity : 55 - 65 %RH

Condition of this results of calibration :

1. This equipment was calibrated by insert 3 standard temperature recorder into its chamber and test according to WI-T23 inhouse method.(based on BS 2646-1 : 2021)
   All data show below were final values and the initial data from customer request . The temperature scale used was based on ITS - 90 .
2. Reference Standard Instrument :

Instrument	Model	Standard No.	Certificate No.	Due Date
1. Temperature recorder	RTD	T210	T242028	11 December 2025
2. Temperature recorder	RTD	T211	T242029	11 December 2025
3. Temperature recorder	RTD	T212	T242030	11 December 2025


3. This certificate is traceable to :
   National Institute of Metrology (Thailand) through Metrological Center (NSC-TISI-TIS 17025 CALIBRATION 0244.)
4. Condition of calibrated item : good
   Equipment Description :
   Pressure Indicator 0.11-0.12 MPa At 121 °C Holding time 20 minute

5. Adjustment :
   (X) without adjustment ( ) after adjustment

Approved By. _____

SCG
Metrology
SCI ECO Services Company Limited
33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110, Thailand.
NSC-TISI-TIS 17025
CALIBRATION 0244

Calibration Report

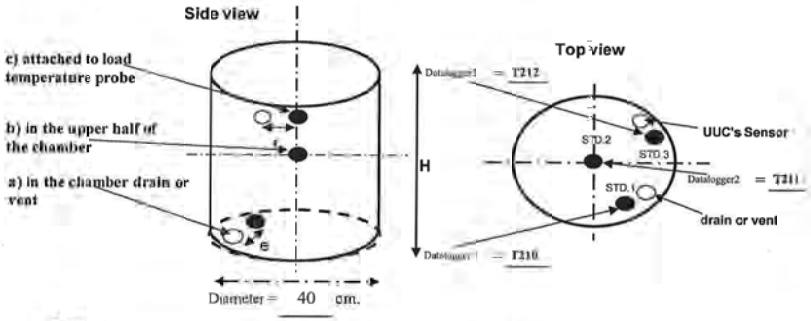

Remark :

Size of Installed Standard sensor STD.1 : Distance the chamber drain or vent e ≤ 10 cm.(less than or be equal to 10 cm.)
Size of Installed Standard sensor STD.2 : Geometric Center (upper half of the chamber)
Size of Installed Standard sensor STD.3 : Distance UUC's Sensor f = 2 cm.

Measurement Results :

	Average Standard Reading at each position (°C)		
Calibration Point	T210	T211	T212
121	121.2	121.1	121.1

Autoclave			Temperature Distribution				
Setting (°C)	Reading (°C)		Average	Stability	Uniformity	Uncertainty	Coverage
	Min , Max	Average	(°C)	(±°C)	(±°C)	(±°C)	Factor *k*
121	-	121	121.2	0.1	0.1	0.65	2.00

* The quoted uncertainty exclude "uniformity"

The calibration result apply only the above calibrated item.

The result of test was found accurate as shown on date and place of test only.


The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor *k* which for a t-distribution, providing a level of confidence of approximately 95 % .

End of Certificate

Approved By._____

Metrological Center
SCG CEMENT-BUILDING MATERIALS
SCI ECO Services Company Limited
33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110
Telephone : +66 2 586 5792-4 Fax : +66 2 586 5109
Website : www.scieco.co.th E-Mail : calibrate@scg.co.th

Calibration Report

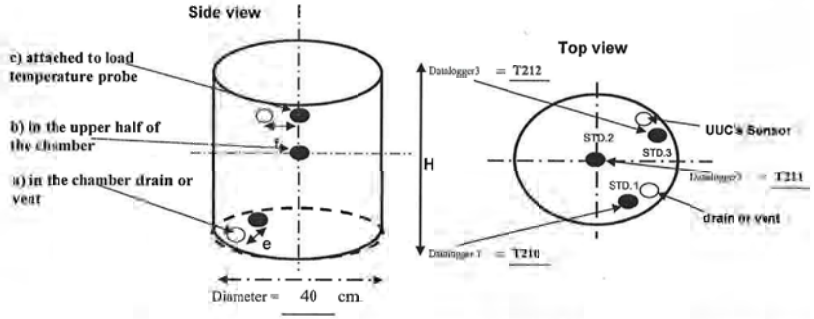

Remark :

Size of Installed Standard sensor STD.1 : Distance the chamber drain or vent e ≤ 10 cm.(less than or be equal to 10 cm.)
Size of Installed Standard sensor STD.2 : Geometric Center (upper half of the chamber)
Size of Installed Standard sensor STD.3 : Distance UUC's Sensor f = 2 cm.

Measurement Results :

	Average Standard Reading at each position (°C)		
Calibration Point	T210	T211	T212
121	121.18	121.12	121.13

Autoclave			Temperature Distribution				
Setting (°C)	Reading (°C)		Average	Stability	Uniformity	Uncertainty	Coverage
	Min , Max	Average	(°C)	(±°C)	(±°C)	(±°C)	Factor *k*
121	-	121	121.16	0.10	0.10	0.65	2.00

* The quoted uncertainty exclude "uniformity"

The calibration result apply only the above calibrated item.

The result of test was found accurate as shown on date and place of test only.

The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor *k* which for a t-distribution, providing a level of confidence of approximately 95 % .

End of Certificate

Approved By._____

TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL.0-2717-3000-29 FAX 0-2719-9484

NSC-TISI-TIS17025 CALIBRATION 0008

Certificate of Calibration

Cert. No.: 24TM1398
Page : 1 of 3

Equipment :	Incubator
Manufacturer :	SHEL-LAB
Model :	1915A
Serial No. :	0200599
ID No. :	BKK_ML0010

REVIEW BY ..... SithichokT.

APPROVED BY.....

NEXT CAL DATE..... 03/12/25

Submitted by : ALS Laboratory Group (Thailand) Co.,Ltd.
104 Phatthanakan 40, Phatthanakan Rd.,
Khwaeng Phatthanakan, Khet Suan Luang,
Bangkok 10250 Thailand

Location : Incubation & Micrological Reading

Received Order : 03 December 2024
Calibration Date : 03 December 2024
Ambient Temperature : (26 ± 10) °C
Relative Humidity : (50 ± 30) %
AC Line Voltage : (220 ± 22) V

Calibrated by : Kunchit Promprat

Approved by :

Approved Signatory

( ) Pornthippa Tameyakul
( ) Ponpan Paipim
(✓) Suwit Imjai

Issue Date : 17 December 2024

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

Procedure Used :-

Calibration were conducted using calibration procedure CP-OT02 based on TLAS G-20 according to direct measurement method with Data Acquisition which connected with Resistance Temperature Detector (RTD).

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-


Instrument	Serial No.	Cert. No.	Traceable	Due Date
1) Data Acquisition	MY49023932	24LM119	TPA	27 Jul 2025

2. This certificate is valid only to the item calibrated on date and place of calibration.
3. This certification is traceable to the International System of Unit.

Remark : TPA : Technology Promotion Association (Thailand - Japan)

Result of Calibration :- (*) Without Adjustment
Function of UUC* : Temperature Source
Fresh air setting : Close

Environment during calibration		
	Beginning	Finished
Temp. (°C)	24	24
REL.Humid. (%)	51	55
AC Supply (Volt)	223	223

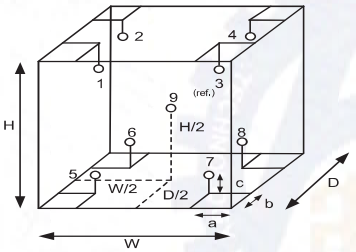

Position :	Ref. Std. ID No.:
1	19-16RTD-01
2	19-16RTD-02
3	19-16RTD-03
4	23-16RTD-04
5	19-16RTD-05
6	19-14RTD-06
7	21-16RTD-07
8	19-16RTD-08
9 (ref.)	19-16RTD-09

Probe Installation Details :

a =	10	cm
b =	10	cm
c =	10	cm

Dimension of Chamber :

D =	0.50	m
W =	0.75	m
H =	1.2	m
Capacity =	0.45	m^3

Equipment : Incubator
Condition As-Received : Used Item
Reference : 2412-0004OC-1
Result of Calibration :- (*) Without Adjustment
Function of UUC* : Temperature Source
Fresh air setting : Close

Calibration Point (°C)	UUC* Setting (°C)	UUC* Reading (°C)	Temperature stability (± °C)	Temperature uniformity (°C)	Overall Variation (°C)	Coverage Factor *k*
35.0	35.0	35.0	0.048	0.40	0.46	2

Calibration Point	Measured Temperature (°C) Position									Uncertainty
(°C)	1	2	3	4	5	6	7	8	9 (ref.)	(±°C)
35.0	34.888	34.840	35.116	35.141	34.750	34.896	34.921	35.054	34.768	0.30

Average* : The average of 30 values in each position.
Temperature stability : One-half of the greatest maximum difference of measured temperature at any one sensor.
Temperature uniformity : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.
Overall Variation : The Difference of the maximum and minimum measured temperatures throughout observation.
UUC* : Unit Under Calibration
Note : The reported uncertainty of measurement was included stability and excluded uniformity .

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor ***k***, providing a level of confidence of approximately 95 %.

-o0o-

TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL.0-2717-3000-29 FAX.0-2719-9484

NSC-TISI-TIS 17025 CALIBRATION 0003

Certificate of Calibration

REVIEW BY SithichokT.
APPROVED BY
NEXT CAL DATE 23/10/25

Equipment : Hot Air Oven
Manufacturer : Binder
Model : ED 240/E2
Serial No. : 00-15533
ID No. : BKK_ML0013
Submitted by : ALS Laboratory Group (Thailand) Co.,Ltd.
104 Phatthanakan 40, Phatthanakan Rd.,
Khwaeng Phatthanakan, Khet Suan Luang,
Bangkok 10250 Thailand
Location : Media Preparation Room

Received Order : 23 April 2024
Calibration Date : 23 April 2024
Ambient Temperature : (26 ± 10) °C
Relative Humidity : (50 ± 30) %

Calibrated by : Tawatchai Pama

Approved by :
Approved Signatory

( ) Ponpan Paipim
(✓) Suwit Imjai
( ) Kunchit Promprat

Issue Date : 26 April 2024

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

Equipment : Hot Air Oven **Cert. No.:** 24TM667
Condition As-Received : Used Item **Page :** 2 of 3
Reference : 2404-0439OC-8

Procedure Used :-

Calibration were conducted using calibration procedure CP-OT02 based on TLAS G-20 according to direct measurement method with Data Acquisition which connected with Thermocouple Type T.

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-


Instrument	Serial No.	Cert. No.	Traceable	Due Date
1) Data Acquisition	MY49001451	24LM44	TPA	17 Mar 2025

2. This certificate is valid only to the item calibrated on date and place of calibration.
3. This certification is traceable to the International System of Unit.

Remark : TPA : Technology Promotion Association (Thailanc - Japan)

Result of Calibration :- (*) Without Adjustment
Function of UUC* : Temperature Source
Fresh air setting : Close

Environment during calibration		
	Beginning	Finished
Temp. (°C)	24	23
REL.Humid. (%)	65	65
AC Supply (Volt)	223	222

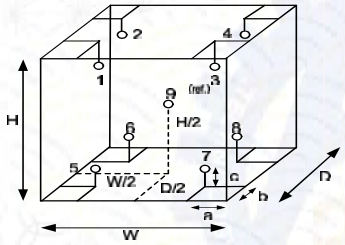

Position :	Ref. Std. ID No.:
1	24-19TC-01
2	24-19TC-02
3	24-19TC-03
4	24-19TC-04
5	24-19TC-05
6	24-19TC-06
7	24-19TC-07
8	24-19TC-08
9 (ref.)	24-19TC-09

Probe Installation Details :

a =	10	cm
b =	10	cm
c =	10	cm

Dimension of Chamber :

D =	0.50	m
W =	0.80	m
H =	0.60	m
Capacity =	0.24	m³

Equipment : Hot Air Oven **Cert. No.:** 24TM667
Condition As-Received : Used Item **Page :** 3 of 3
Reference : 2404-0439OC-8
Result of Calibration :- (*) Without Adjustment
Function of UUC* : Temperature Source
Fresh air setting : Close

Calibration Point (°C)	UUC* Setting (°C)	UUC* Reading (°C)	Temperature stability (± °C)	Temperature uniformity (°C)	Overall Variation (°C)	Coverage Factor *k*
180	180	180	0.64	2.7	3.7	2

Calibration Point (°C)	Measured Temperature (°C) Position									Uncertainty (±°C)
	1	2	3	4	5	6	7	8	9 (ref.)	
180	181.009	181.511	180.922	181.359	181.217	183.659	181.664	181.986	181.474	1.5

Average* : The average of 30 values in each position.
Temperature stability : One-half of the greatest maximum difference of measured temperature at any one sensor.
Temperature uniformity : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or horrogeneity within the chamber under steady-state conditions.
Overall Variation : The Difference of the maximum and minimum measured temperatures throughout observation.
UUC* : Unit Under Calibration
Note : The reported uncertainty of measurement was included stability and excluded uniformity .

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor ***k***, providing a level of confidence of approximately 95 %.

-o0o-

TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL.0-2717-3000-29 FAX.0-2719-9484

NSC-TISI-TIS17025
CALIBRATION 0008

Certificate of Calibration

Cert. No.: 25TM460
Page : 1 of 3

REVIEW BY ..... Sithichok T.

APPROVED BY.....

NEXT CAL DATE..... 04/03/26

Equipment :	Water Bath
Manufacturer :	Memmert
Model :	WNE 45
Serial No. :	L712.0429
ID No. :	BKK_ML0056
Submitted by :	ALS Laboratory Group (Thailand) Co.,Ltd. 104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan, Khet Suan Luang, Bangkok 10250 Thailand
Location :	Incubation & Microbiological Reading
Received Order :	04 March 2025
Calibration Date :	04 March 2025
Ambient Temperature :	(26 ± 10) °C
Relative Humidity :	(50 ± 30) %
AC Line Voltage :	(220 ± 22) V
Calibrated by :	Khit Ruttanaprapachai
Approved by :	Kunchit

Approved Signatory

( ) Chakrit Waewwanjua
( ) Suwit Imjai
(✓) Kunchit Promprat

Issue Date : 06 March 2025

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

Procedure Used :-

Calibration were conducted using in-house calibration procedure CP-OT04 Based on ASTM E715 according to direct measurement method with Data Acquisition which connected with Industrial Platinum Resistance Thermometer (IPRT).

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-


Instrument	Serial No.	Cert. No.	Traceable	Due Date
1) Data Acquisition	MY44073381	23LM73	TPA	18 May 2025

2. This certificate is valid only to the item calibrated on date and place of calibration.
3. This certification is traceable to the International System of Unit.

Remark : TPA : Technology Promotion Association (Thailand - Japan)

Result of Calibration :- (*) Without Adjustment
Function of UUC* : Temperature Source
Heat transfer medium used : Water

	Environmental		AC Voltage Supply
	(°C)	(%R.H.)	(Volt)
Beginning of Calibration	24	49	220
Finished of Calibration	25	51	221

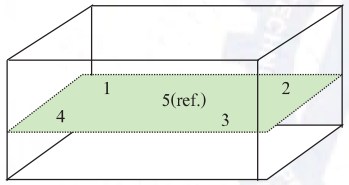

Front

Position :	Ref. Std. S/N.:
1	4803988-006
2	4803988-007
3	4804539-014
4	4804539-015
5(ref.)	4804539-016

Equipment : Water Bath
Condition As-Received : Used Item
Reference : 2503-0006OC-2
Result of Calibration :- (*) Without Adjustment
Function of UUC* : Temperature Source

Cert. No.: 25TM460
Page : 3 of 3

Calibration point (°C)	UUC* Setting (°C)	UUC* Reading (°C)	Average* Standard Reading (°C) Position					Uncertainty (± °C)
			1	2	3	4	5 (ref.)	
44.5	44.5	44.5	44.489	44.469	44.497	44.476	44.479	0.15
45.0	45.0	45.0	44.990	44.966	44.997	44.983	44.980	0.15

Calibration point (°C)	Uniformity (°C)	Stability (± °C)	Coverage Factor *k*
44.5	0.045	0.035	2
45.0	0.047	0.031	2

Average* : The average of 30 values in each position.
Uniformity : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.
Stability : One-half of the greatest maximum difference of measured temperature at any one probe.
UUC* : Unit Under Calibration
Note : The reported uncertainty of measurement was included stability and excluded uniformity.

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor ***k***, providing a level of confidence of approximately 95 %.

-o0o-

REVIEW BY
APPROVED BY
NEXT CAL. DATE 13/08/25

HACH
Be Right

Test Report

Customers	:	ALS Laboratory Group (Thailand) Co., Ltd.			
Equipment	:	Colorimeter	Manufacturer	:	HACH
Controller Model	:	☑ DR300 ☐ Pocket II	ID No.	:	BKK_LG0040
Controller Serial No.	:	190500A000330	Sensor Serial No.	:	-
Date of Test	:	13/08/2024	Period	:	1 Year
Environment temperature	:	25 °C	Humidity	:	50 %RH

Results

Instrument Checked

Item	Characteristic	Before		After		Remark
1	Visual Inspect	☑ Pass	☐ Fail	☑ Pass	☐ Fail	
2	Power Supply (4.5 – 6.0 VDC)	6.0	VDC	6.0	VDC	
3	Display Check	☑ Pass	☐ Fail	☑ Pass	☐ Fail	
4	Keyboard Check	☑ Pass	☐ Fail	☑ Pass	☐ Fail	
5	Function System Program	☑ Pass	☐ Fail	☑ Pass	☐ Fail	

Warning and Error Checked

Item	Event	Before	After
6	Error list	☑ None ☐ Appear	☑ None ☐ Appear

Check with Standard

Item	Characteristic	Before	After	Remark
	DPD CHLORINE-LR			
7	Blank (0.00 mg/l)	0.00 mg/l	0.00 mg/l	
8	Standard Cl2 No. 1 (0.19 ± 0.38 mg/l)	0.21 mg/l	0.20 mg/l	
9	Standard Cl2 No. 2 (0.87 ± 0.10 mg/l)	0.89 mg/l	0.88 mg/l	
10	Standard Cl2 No. 3 (1.55 ± 0.14 mg/l)	1.57 mg/l	1.55 mg/l	
	DPD CHLORINE-HR			
11	Blank (0.0 mg/l)	0.0 mg/l	0.0 mg/l	
12	Standard Cl2 No. 1 (2.2 ± 0.2 mg/l)	2.2 mg/l	2.2 mg/l	
13	Standard Cl2 No. 2 (3.9 ± 0.3 mg/l)	3.9 mg/l	3.9 mg/l	
14	Standard Cl2 No. 3 (6.8 ± 0.6 mg/l)	6.8 mg/l	6.8 mg/l	

บริษัท ฮัค (ประเทศไทย) จำกัด, อาคารสินสาธร ๒ ชั้นที่ ๑๑ ห้องเลขที่ ๑๑๐๔ ถนนสาทรใต้ แขวงยานนาวา เขตสาทร กรุงเทพฯ ๑๐๑๒๐
Tel: +66 (02) 026-8529 | Fax: +66(02) 026-3572 | Tax ID : 0105521073301 | Email: thmarketing@hach.com | www.th.hach.com

HACH
Be Right™

Summary of checked

- ☑ The instrument can work normally and efficiently. (เครื่องมือวัดสามารถทำงานได้ปกติและมีประสิทธิภาพ)
- ☐ The instrument can work but it's requiring to maintenance. (เครื่องมือวัดสามารถทำงานได้แต่ต้องบำรุงรักษา)
- ☐ The instrument could not work it's requiring to repair. (เครื่องมือวัดไม่สามารถทำงานได้และต้องการซ่อมบำรุง)

Remark:

Standard Equipment Used

Equipment	Equipment I.D.	
Standard Absorbance DPD-CHLORINE-LR	Lot No. A3020	Exp. date : Feb-25
Standard Absorbance DPD-CHLORINE-HR	Lot No. A4025	Exp. date : Jan-26
Digital multi meter	S/N : 19430618	Due date : Oct-24
Thermo hygrometer	S/N : 34855953	Due date : Oct-24

Test By : WILAILAK S.
(Miss Wilailak Sawangpan)
Service Engineer

Approved by :
(Mr. Suanun Sartyangkool)
Position : Assistant Service Division Manager

บริษัท ฮัค (ประเทศไทย) จำกัด: อาคารซี ห้องเลขที่ ซี 3 11 ชั้นที่3 เลขที่ 735/4 คอมเพล็กซ์ กรุงเทพฯ 10250
Tel: +66 (02) 026-3529 | Fax: +66(02) 026-3572 | Tax ID : 0105552107330 | Email: thmarketing@hach.com | www.th.hach.com

REVIEW BY Autchaiawan S.
APPROVED BY Tanyatorn M.
NEXT CAL. DATE ~~12 Jan 2025~~ 12 Jul 2025

ARCHEMICA

Certificate of Calibration

ICS-2100: Anion (ID#659)

This certificate is to verify that instrument below are calibrated

by Archemica Lab Co., Ltd.

ICS-2100 S/N: 15010977

AS-HV S/N: 5450A36659

For

ALS Laboratory Group (Thailand) Co., Ltd.

บริษัท อาร์เคมีก้า แลบ จำกัด
ARCHEMICA LAB CO.,LTD.

Operator Signature: Nutdanai Date: Jan 12, 2024

(Mr.Nutdanai Laekhwan)

Application Chemist

SCIMET

SCIMET Co., Ltd.
1194 Soi Wachirathamsathit 57, Bangchak,
Phrakhanong, Bangkok 10260 Thailand
Email:scimet2022@gmail.com, Tel: 02 460 9239
https://www.scimet.co.th

ilac-MRA

NSC-TISI-TIS 17025
CALIBRATION 0454

Certificate No. C07240192

Calibration Certificate

Equipment:	SPECTROPHOTOMETER		
Model:	DR 3900	Job No.:	KSMT2403543
Serial No.(or ID):	2403637	Received Date:	25 December 2024
Manufacturer:	HACH	Issued Date:	25 December 2024
Condition:	New	Page:	1 of 3

REVIEW BY Ananta B.
APPROVED BY Kanitta H.
NEXT CAL. DATE 25/12/25

Customer

ALS Laboratory Group (Thailand) Co., Ltd
114/1 Moo 8, Karnchanawanich Rd.T. Ban Phru, A Hatyai, Songkhla 90250

Calibration Place

Hach (Thailand) Limited.
Branch 00001, Building D Room No. D3 11, 3rd Floor, No. 735/4, Srinakarin Road,
Pattanakarn, Suanluang, Bangkok 10250 Thailand.

Calibration Date

25 December 2024

Environment Condition

Temperature: 22.2 °C ± 0.5 °C
Humidity: 59.2 %RH ± 2.3 %RH

The Method used

In-house method, WI07, based on ASTM E 275-08 and
ASTM E 387-04

Traceability

This certificate is traceable to the CRM maintained by National Institute of Standards and Technology (NIST) through Starna Scientific Limited.

The standard for Wavelength Certificate No. 108691 and 108692

The standard for Photometric Certificate No. 109010 , 114655

This certificate is issued the units of measurement according to the International System of Units (SI). It provides traceability of measurement to international or national standard or other recognized national standard laboratories.

The measurement uncertainty stated is the expanded uncertainty which is obtained from the standard uncertainty multiplied by the coverage factor (k=2) to provide a level of confidence of approximately 95%. It is determined in accordance with the Guide to Expression of Uncertainty in Measurement (GUM).

These results may be affected by deviations from specified conditions. The results relate only to the items tested, calibrated or sampled. The report shall not be reproduced except in full without approval of SCIMET Co., Ltd.

(Mr. Siwapan Srijan)
Person in charge

SCIMET CO.,LTD

(Mr. Thalerngkeat Poungngam)
Authorized signatory

SCIMET

Condition of reference standards Instruments / CRM:

Instruments	Set No.	Certificate No.	Due date
Holmium Oxide Glass Reference	121512	108691	25-Jan-25
Didymium Oxide Glass Reference	119722	108692	25-Jan-25
Neutral Density Filter Reference	12276	109010 , 114655	2-Feb-25

Calibration Results:

Without Adjustment

Wavelength Accuracy (nm), The spectral bandwidth of Std at 5 nm and UUC at 5 nm

Standard Wavelength (nm)	Unit Under Calibration (nm)	Correction (nm)	Uncertainty of Measurement (± nm)
333.67	333	0.67	0.59
361.02	361	0.02	0.59
417.80	417	0.80	0.59
441.29	441	0.29	0.59
479.88	480	-0.12	0.59
513.75	513	0.75	0.59
528.59	528	0.59	0.59
537.75	537	0.75	0.59
585.56	585	0.56	0.59
641.95	642	-0.05	0.59
684.70	685	-0.30	0.59
747.61	748	-0.39	0.59
807.04	807	0.04	0.59
879.68	880	-0.32	0.59

บริษัท ซายน์เมท จำกัด (SCIMET CO., LTD.)
1194 Soi Wachirathamsathit 57, Bangchak, Phrakhanong, Bangkok 10260 Thailand
Email: scimet2022@gmail.com, Tel: 02 460 9239

Calibration Results:

Without Adjustment

Photometric Accuracy (Absorbance)

Wavelength	Standard absorbance (Abs)	Unit Under Calibration (Abs)	Correction (Abs)	Uncertainty of Measurement(± Abs)
420 nm	0.0000	0.000	0.0000	0.0045
	0.2373	0.234	0.0033	0.0045
	0.5617	0.561	0.0007	0.0045
	0.7392	0.738	0.0012	0.0045
	1.0550	1.056	-0.0010	0.0045
440 nm	0.0000	0.000	0.0000	0.0045
	0.2335	0.231	0.0025	0.0045
	0.5513	0.550	0.0013	0.0045
	0.7230	0.722	0.0010	0.0045
	1.0324	1.032	0.0004	0.0045
465 nm	0.0000	0.000	0.0000	0.0045
	0.2126	0.210	0.0026	0.0045
	0.5036	0.506	-0.0024	0.0045
	0.6735	0.676	-0.0025	0.0045
	0.9615	0.965	-0.0035	0.0045
546.1 nm	0.0000	0.000	0.0000	0.0045
	0.2201	0.217	0.0031	0.0045
	0.5176	0.520	-0.0024	0.0045
	0.6930	0.694	-0.0010	0.0045
	0.9908	0.994	-0.0032	0.0045
590 nm	0.0000	0.000	0.0000	0.0045
	0.2443	0.241	0.0033	0.0045
	0.5530	0.554	-0.0010	0.0045
	0.7196	0.719	0.0006	0.0045
	1.0301	1.031	-0.0009	0.0045
635 nm	0.0000	0.000	0.0000	0.0045
	0.2646	0.261	0.0036	0.0045
	0.5370	0.538	-0.0010	0.0045
	0.6862	0.687	-0.0008	0.0045
	0.9822	0.984	-0.0018	0.0045

The End of Certificate

บริษัท ซายน์เมท จำกัด (SCIMET CO., LTD.)
1194 Soi Wachirathamsathit 57, Bangchak, Phrakhanong, Bangkok 10260 Thailand
Email: scimet2022@gmail.com, Tel 02 460 9239