



JIRANATEE ASSOCIATES CO.,LTD.

Jiranatee Associates Co.,Ltd.
63/14-15, 67/35-36
Petchkasem 7,7/1, Rd.Watthapra, Bangkokyai,
Bangkok 10600 (Thailand)
Tel: +6608680812
Mobile: +66863999453
E-mail: jnac-calibration@jiranatee.com
Web site: www.jiranatee.com

Accredited calibration laboratory
ISO/IEC 17025:2017
NSC-TISI-TIS 17025
CALIBRATION 0367

Flow measurement laboratory
Calibration services department.



CERTIFICATE OF CALIBRATION

Certificate No. : COF-044-67

Page 1 of 2 Pages

MEASUREMENT ITEM : Top Load Orifice
MANUFACTURER : TISCH
MODEL/TYPE : TE-5028
SERIAL NUMBER : 3945
ID NUMBER : TNP-F-CAL02
CONDITION AS-RECEIVED : Used item
CUSTOMER : TNP Environment Co., Ltd.
332/173 Vision Smart Life Village, Bangrak Phatthana,
Bang Bua Thong District, Nonthaburi 11110

RECEIVED DATE : 29 Oct 2024
MEASUREMENT DATE : 30 Oct 2024
ISSUE DATE : 30 Oct 2024

ENVIRONMENTAL CONDITIONS:

Ambient condition in the laboratory are as follow:

Temperature	: 23.0 ± 3.0	°C
Relative Humidity	: 55.0 ± 15.0	%RH
Atmospheric Pressure	: 1010 ± 10	hPa

CALIBRATION CONDITION:

Preconditioning : 24 hours at ambient conditions.
Measurement Condition : The average values during measurement are 23.9 °C and 55.8 %RH.

NOTED: The certificate is valid only to the item calibrated on date and place of calibration.

TABULATION OF RESULTS:

The table on next page give the measured values.

Calibration procedure:

The Orifice gas flow device was calibrated against Standard Rotary Displacement Meter (Roots Meter) Model G65/IMC/W2-dp. The WI-CL-004 was used as a calibration guideline.

Traceability:

This certificate provides a traceability of the measurement to recognized the national standards, and to realization of the international system of units (SI) through the NIMT (National Metrology Institute of Thailand) via Certificate number: MW-0063-23.

Uncertainty of Measurement:

The reported uncertainty of measurement is based on the standard uncertainty multiplied by a coverage factor $k=2$, Which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty has been determined in accordance with the GUM 'Evaluation of measurement data - Guide to the expression of uncertainty in measurement'

Calibrated by:



MEASUREMENT RESULTS:

The Orifice gas flow device was calibrated by direct comparison method with the Standard Rotary Displacement Meter (Roots Meter). The Humid air was used as a medium in the system. The standard conditions are 25°C (298.15 K) and 760 mmHg for standard temperature and standard pressure respectively.

Table 1: The results of Q Standard calibration data

Plate	Flow rate m^3/min	Pressure [Pa] mmHg	Temperature [Ta] °C	Temperature [Tm] °C	Δp_{meter} mmHg	$\Delta p_{Orifice}$ inH ₂ O	Y	Standard Flow [Q_s] m^3/min
1	0.703	758.163	23.78	22.67	49.921	1.158	1.077	0.660
2	0.999	758.204	23.26	22.30	35.795	2.480	1.577	0.959
3	1.117	758.225	23.29	22.38	30.579	3.143	1.776	1.079
4	1.164	758.281	23.31	22.57	28.519	3.425	1.854	1.127
5	1.414	758.199	23.33	22.86	18.318	5.237	2.292	1.387

Slope (m): 1.66978
 Intercept (b): -0.02500
 Correlation coefficient (r): 0.99989
 Uncertainty ($k=2$): 0.015 m^3/min

Table 2: The results of Q actual calibration data

Plate	Flow rate m^3/min	Pressure [Pa] mmHg	Temperature [Ta] °C	Temperature [Tm] °C	Δp_{meter} mmHg	$\Delta p_{Orifice}$ inH ₂ O	Y	Standard Flow [Q_a] m^3/min
1	0.703	758.163	23.78	22.67	49.921	1.158	0.673	0.659
2	0.999	758.204	23.26	22.30	35.795	2.480	0.985	0.955
3	1.117	758.225	23.29	22.38	30.579	3.143	1.109	1.075
4	1.164	758.281	23.31	22.57	28.519	3.425	1.157	1.123
5	1.414	758.199	23.33	22.86	18.318	5.237	1.431	1.382

Slope (m): 1.04588
 Intercept (b): -0.01565
 Correlation coefficient (r): 0.99989
 Uncertainty ($k=2$): 0.015 m^3/min

End of Certificate of Calibration



Analyzer Performance Test

Calibrated Date: 08 November 2024

Instruments Information

Analyzer Type : CO Analyzer

Model : 48C

Manufacturer : Thermo Environmental

Serial Number : 48C-67530-357

Calibrator Unit

Dilutor Model : Dasibi Model 5008

Serial Number : 705

ZERO AIR Generator : API MODEL 701

Serial Number : 1924

Standard Gas Concentration

Nitric Oxide (NO) 55.47 PPM

Sulphur Dioxide (SO₂) 55.11 PPM

Carbon Monoxide (CO) 4,535 PPM


Cylinder number EB0129027

Expire Date: 29 Oct. 2027

Environment : Temperature 25.5 °C Humidity: 51 %RH

Calibration Report

	Zero			Span		
	Reference (PPM)	Reading (PPM)	Drift (PPM)	Reference (PPM)	Reading (PPM)	Drift%
Before	0.0	0.2	0.2	45.0	44.2	-1.8
After	0.0	0.0	0.0	45.0	45.0	0.0

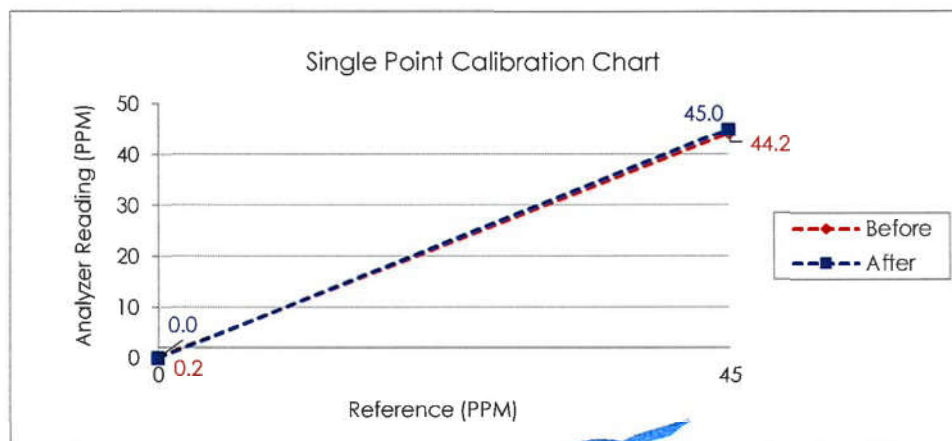

Calibrate By :

Analyzer Performance Test

Calibrated Date: 13 September 2024

Instruments Information

Analyzer Type : CO Analyzer
Model : 48C

Manufacturer : Thermo Environmental
Serial Number : 0401204259

Calibrator Unit

Dilutor Model : Dasibi Model 5008
Serial Number : 705
ZERO AIR Generator : API MODEL 701
Serial Number : 1924


Standard Gas Concentration

Nitric Oxide (NO) 55.47 PPM
Sulphur Dioxide (SO₂) 55.11 PPM
Carbon Monoxide (CO) 4,535 PPM
Cylinder number EB0129027
Expire Date: 29 Oct. 2027


Environment : Temperature 25.5 °C Humidity: 51 %RH

Calibration Report

	Zero			Span		
	Reference (PPM)	Reading (PPM)	Drift (PPM)	Reference (PPM)	Reading (PPM)	Drift%
Before	0.0	0.2	0.2	45.0	44.3	-1.7
After	0.0	0.0	0.0	45.0	45.0	0.0

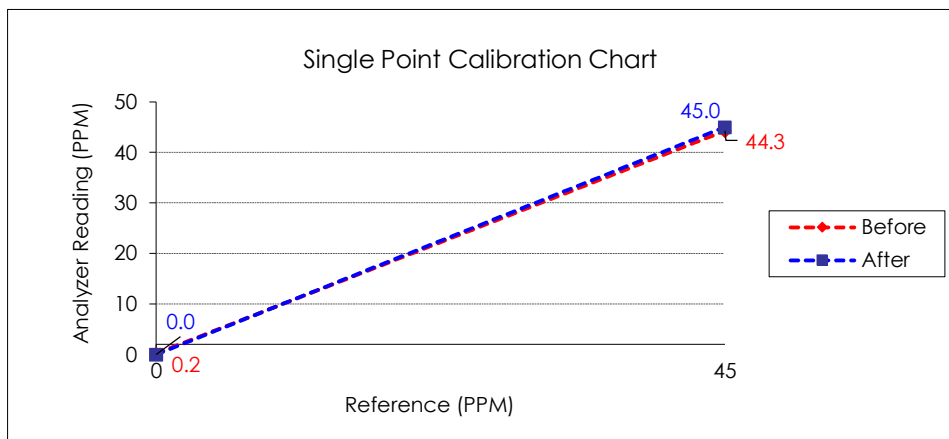

Calibrate By :





บริษัท เอ็นไวร์ เซอร์วิส จำกัด

บริษัท เอ็นไวร์ เซอร์วิส จำกัด
ENVIR SERVICE CO., LTD.

42 รามอินทรา 14 แยก 9 แขวงท่าแร้ง เขตบางเขน กรุงเทพฯ 10230 โทรศัพท์ 02-9435814-5 โทรสาร 02-9438201
42 Raminthra 14 yeak 9, Tha Rang, Bangkhen, Bankok 10230 Tel : 02-9435814-5 Fax : 02-9438201

Analyzer Performance Test

Calibrated Date: 14 August 2024

Instruments Information

Analyzer Type: NO/NO2/NOx Analyzer Model: 42C	Manufacturer Thermo Environmental S/N: 42C-56817-311
--	---

Calibration System

Calibrator Unit	Standard Gas
Dilutor Model Dasibi Model 5008 S/N: 705 ZERO AIR Generator API Model 701 S/N: 1924	NO Conc 55.47 PPM SO2 Conc 55.11 PPM CO Conc 4,535 PPM Cylinder number EB0129027 Expire Date: 29 Oct. 2027

Environment: Temperature 25.5 °C


Humidity: 51 %RH

Calibration Check (Before adjust)

GAS	Zero			Span		
	Reading Value (ppb)	Expected Value (ppb)	Drift (ppb)	Reading Value (ppb)	Expected Value (ppb)	Drift%
NO	0.1	0.0	0.1	393.3	400.0	-1.7
NOx	0.1	0.0	0.1	396.5	400.0	-0.9

Calibration Check (After adjust)

GAS	Zero			Span		
	Reading Value (ppb)	Expected Value (ppb)	Drift (ppb)	Reading Value (ppb)	Expected Value (ppb)	Drift%
NO	0.0	0.0	0.0	400.0	400.0	0.0
NOx	0.0	0.0	0.0	400.0	400.0	0.0

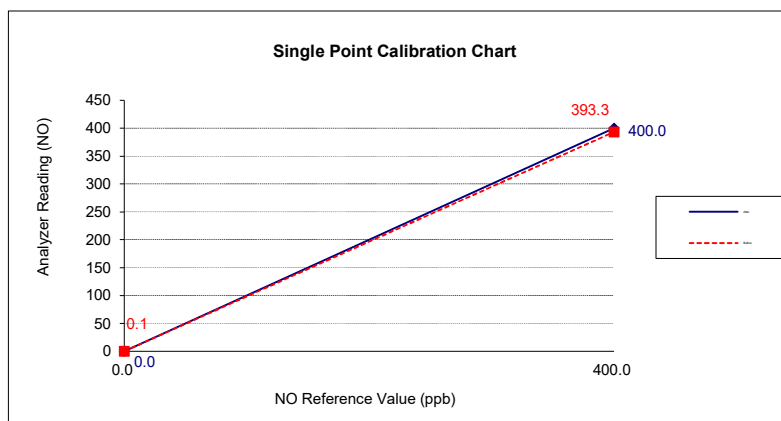

Analyzer Performance Test

Calibrated Date: 14 August 2024

Instruments Information

Analyzer Type : NO-NO2-NOx Analyzer

Manufacturer : Thermo Environmental

Model : 42C

Serial Number : 42C-59194-321

Calibrator Unit

Dilutor Model : Dasibi Model 5008

Serial Number : 705

ZERO AIR Generator : API MODEL 701

Serial Number : 1924

Standard Gas Concentration

Nitric Oxide (NO) 55.47 PPM

Sulphur Dioxide (SO2) 55.11 PPM

Carbon Monoxide (CO) 4,535 PPM

Cylinder number EB0129027

Expire Date: 29 Oct. 2027


Environment : Temperature 25.5 °C Humidity: 51 %RH

Calibration Report (Before Adjust)

Status	Zero			Span		
	Reference (PPB)	Reading (PPB)	Drift (PPB)	Reference (PPB)	Reading (PPB)	Drift%
NO	0.0	0.1	0.1	400.0	393.3	-1.7
NOx	0.0	0.0	0.0	400.0	393.6	-1.6

Calibration Report (After Adjust)

Status	Zero			Span		
	Reference (PPB)	Reading (PPB)	Drift (PPB)	Reference (PPB)	Reading (PPB)	Drift%
NO	0.0	0.1	0.1	400.0	400.0	0.0
NOx	0.0	0.0	0.0	400.0	400.0	0.0

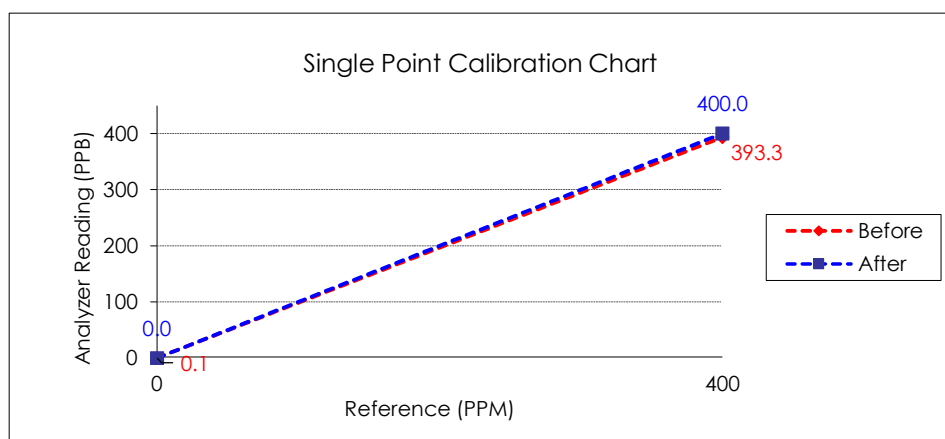

Calibrate By :

Analyzer Performance Test

Calibrated Date: 26 September 2024

Instruments Information

Analyzer Type : SO2 Analyzer

Manufacturer : Thermo Environmental

Model : 43C

Serial Number : 0433609337

Calibrator Unit

Dilutor Model : Dasibi Model 5008

Serial Number : 705

ZERO AIR Generator : API MODEL 701

Serial Number : 1924

Standard Gas Concentration

Nitric Oxide (NO) 55.47 PPM

Sulphur Dioxide (SO₂) 55.11 PPM

Carbon Monoxide (CO) 4,535 PPM


Cylinder number EB0129027

Expire Date: 29 Oct. 2027


Environment : Temperature 25.5 °C Humidity: 51 %RH

Calibration Report

Status	Zero			Span		
	Reference (PPB)	Reading (PPB)	Drift (PPB)	Reference (PPB)	Reading (PPB)	Drift%
Before	0.0	0.1	0.1	400.0	393.4	-1.7
After	0.0	0.0	0.0	400.0	400.0	0.0

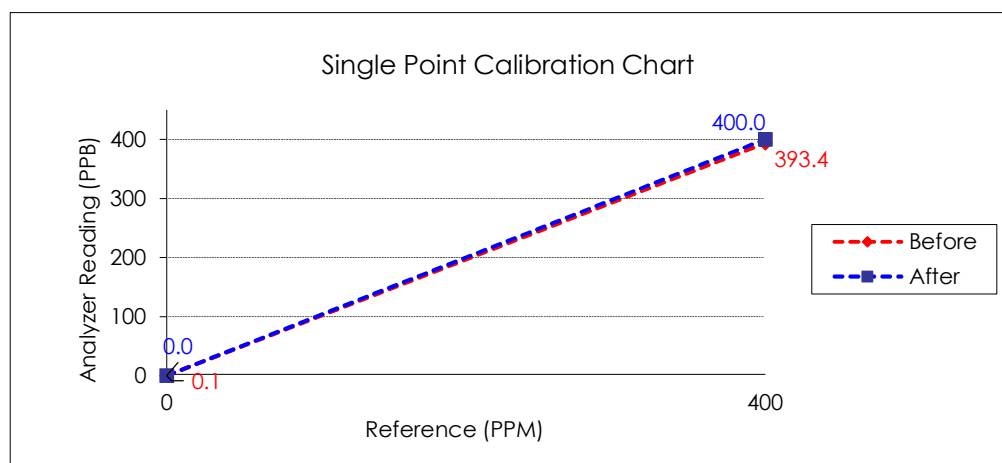

Calibrate By :



Analyzer Performance Test

Calibrated Date: 07 November 2024

Instruments Information

Analyzer Type : SO₂ Analyzer
Model : 43C

Manufacturer : Thermo Environmental
Serial Number : 43C-0427408948

Calibrator Unit

Dilutor Model : Dasibi Model 5008
Serial Number : 705
ZERO AIR Generator : API MODEL 701
Serial Number : 1924


Standard Gas Concentration

Nitric Oxide (NO) 55.47 PPM
Sulphur Dioxide (SO₂) 55.11 PPM
Carbon Monoxide (CO) 4,535 PPM
Cylinder number EB0129027
Expire Date: 29 Oct. 2027

Environment : Temperature 25.5 °C Humidity: 51 %RH

Calibration Report

Status	Zero			Span		
	Reference (PPB)	Reading (PPB)	Drift (PPB)	Reference (PPB)	Reading (PPB)	Drift%
Before	0.0	0.1	0.1	400.0	393.2	-1.7
After	0.0	0.0	0.0	400.0	400.0	0.0

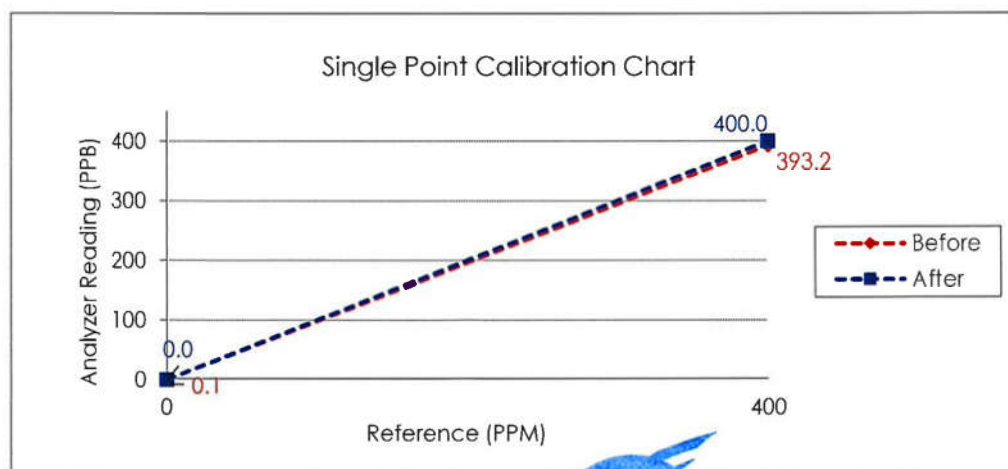

Calibrate By :



Analyzer Performance Test

Calibrated Date: 2023-Nov-1

Instruments Information

Analyzer Type : CH4-NMHC-THC Analyzer

Manufacturer : HORIBA

Model : APHA-360CE

Serial Number : 423740300209

Calibrator Unit

Dilutor Model : Dasibi Model 5008

Serial Number : 705

ZERO AIR Generator : API MODEL 701

Serial Number : 1924

Standard Gas Concentration

Methane (CH₄) 181.0 PPM

Propane 180.7 PPM

Cylinder number EB0123130

Expire Date: 3 Oct. 2027


Environment : Temperature 25.5 °C Humidity: 51 %RH

Calibration Report (Before adjust)

Status	Zero			Span		
	Reference (PPM)	Reading (PPM)	Drift (PPM)	Reference (PPM)	Reading (PPM)	Drift%
Methane	0.0	0.1	0.1	50.0	49.1	-1.8
NMHC	0.0	0.1	0.1	50.0	48.9	-2.2

Calibration Report (After adjust)

Status	Zero			Span		
	Reference (PPM)	Reading (PPM)	Drift (PPM)	Reference (PPM)	Reading (PPM)	Drift%
Methane	0.0	0.0	0.0	50.0	50.0	0.0
NMHC	0.0	0.0	0.0	50.0	50.0	0.0

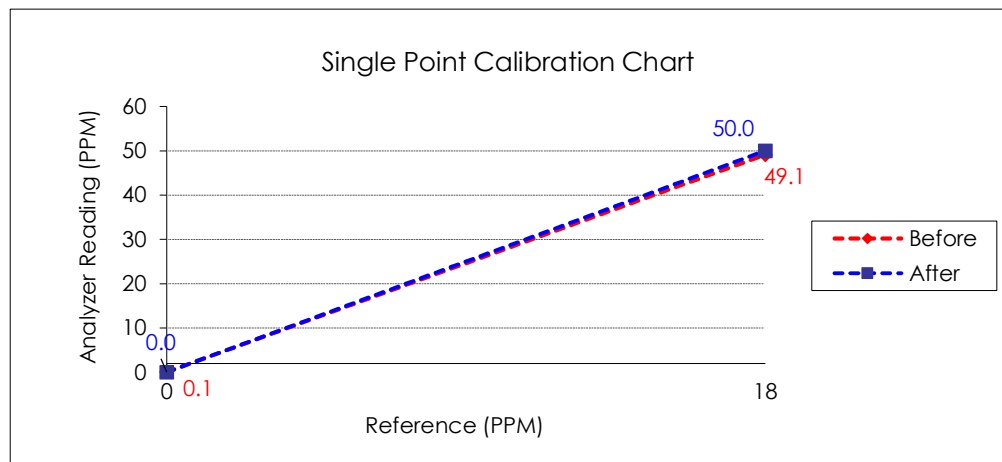

Calibrate By :



THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-67/0575

MTC No. EEL. BP. 15/0867

CALIBRATION CERTIFICATE

Submitted by : TNP ENVIRONMENT CO.,LTD.

Address : 332/173 Moo 3 Bang Rak Phatthana, Bang Bua Tong, Nonthaburi 11110.

Calibrated at : Electrical and Electronic Standards Laboratory, Industrial Metrology and Testing Service Centre.
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Rd., Muang, Samutprakan 10280.

Instrument Calibrated :

Description : Sound Calibrator

Manufacturer : KEPLER

Model : KSM-42C

Serial No. : 160100568

Ambient Environment

Temperature : $(23 \pm 3) ^\circ\text{C}$

Relative Humidity : $(50 \pm 15) \%$

Ambient Pressure : $(101.325 \pm 1.500) \text{ kPa}$

Standards used : 1. Digital Function Synthesizer NF Electronic DF-193A S/N 122037.

2. Measuring Amplifier Bruel&Kjaer 2636 S/N 1537484.

3. Programmable Attenuator Tamagawa TPA-303A S/N OF 2214.

4. Digital Multimeter Agilent 34401A S/N MY44005560.

5. Pressure Transmitter Vaisala PTB202AD S/N T0650001.

6. Audio Analyzer Panasonic VP-7722A S/N 041477D122.

7. Condenser Microphone B&K 4180 S/N 2633526.

Calibration Procedure: CP-102-04 based on IEC 60942-2003. The sound pressure level of instrument was measured by standard microphone using an insert voltage technique.

This instrument has been calibrated against standards maintained at Electrical and Electronic Standards Laboratory (EEL), which are traceable to the International System of Units through the National Institute of Metrology (Thailand).

The information on actual reading is attached herewith and the uncertainty limits quoted refer to the measured values only.

Date of Receipt : 6 Aug. 2024

Date of Calibration : 26 Aug. 2024

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.5

Head Office

35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9009

Office/Laboratory

668 Mu 2 Tambon Bangpoomai, Amphoe Muang Samutprakan,
Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtc@tistr.or.th Website : www.tistr.or.th

Office

196 Phahonyothin Road, Ladyao, Chatuchak,
Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827

THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-67/0575

MTC No. EEL. BP. 15/0867

The reported expanded uncertainty is based upon a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%.

Nominal Output of Unit Under Test = 94 dB re 20 μ Pa at 1000 Hz

Acoustic Output in dB re 20 μ Pa , Corrected to Reference Conditions : 101.325 kPa , 23.0°C and 50 %RH

1. Sound Pressure Level

Standard Microphone Type	Measured Sound Pressure Level (dB)	Deviated value (dB)	Uncertainty (dB)	Tolerance limit IEC60942:2003 Class 2
1/2 inch Bruel&Kjaer 4180	94.30	0.30	± 0.10	± 0.75 dB

2. Frequency

Standard Microphone Type	Measured Frequency (Hz)	Deviated value (Hz)	Uncertainty (Hz)	Tolerance limit IEC60942:2003 Class 2
1/2 inch Bruel&Kjaer 4180	969.9	-30.1	± 1.5	$\pm 2.0\%$

3. Total distortion

Standard Microphone Type	Measured Total distortion (%)	Uncertainty (%)	Tolerance limit IEC60942:2003 Class 2
1/2 inch Bruel&Kjaer 4180	1.70	± 0.50	$\pm 4.0\%$

Note : 1. No adjustment.

2. The calibrator pressure correction was not included.

3. The microphone volume correction was not included.

Date of Calibration : 26 Aug. 2024

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.5

Head Office

35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand

Tel. (66) 0 2577 9036

Fax. (66) 0 2577 9009

Office/Laboratory

668 Mu 2 Tambon Bangpoomai, Amphoe Muang Samutprakan,
Changwat Samutprakan 10280, Thailand

Tel. (66) 0 2323 1672-80 ext. 115, 116

(66) 08 3219 9440

E-mail : mtc@tistr.or.th Website : www.tistr.or.th

Office

196 Phahonyothin Road, Ladyao, Chatuchak,
Bangkok 10900, Thailand

Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217

(66) 08 1889 6827

THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-67/0575

MTC No. EEL. BP. 15/0867

Nominal Output of Unit Under Test = 114 dB re 20 μ Pa at 1000 Hz

Acoustic Output in dB re 20 μ Pa , Corrected to Reference Conditions : 101.325 kPa , 23.0 °C and 50 %RH

1. Sound Pressure Level

Standard Microphone Type	Measured Sound Pressure Level (dB)	Deviated value (dB)	Uncertainty (dB)	Tolerance limit IEC60942:2003 Class 2
1/2 inch Bruel&Kjaer 4180	114.33	0.33	± 0.10	± 0.75 dB

2. Frequency

Standard Microphone Type	Measured Frequency (Hz)	Deviated value (Hz)	Uncertainty (Hz)	Tolerance limit IEC60942:2003 Class 2
1/2 inch Bruel&Kjaer 4180	965.6	-34.4	± 1.5	$\pm 2.0\%$

3. Total Distortion


Standard Microphone Type	Measured Total Distortion (%)	Uncertainty (%)	Tolerance limit IEC60942:2003 Class 2
1/2 inch Bruel&Kjaer 4180	2.15	± 0.50	$\pm 4.0\%$

Note : 1. No adjustment.

2. The calibrator pressure correction was not included.

3. The microphone volume correction was not included.

Calibrated by :



Approved by :


for (Mr. Prawate Kluaypa)

Director

Electrical and Electronic Standards Laboratory

Industrial Metrology and Testing Service Centre

Date of Calibration : 26 Aug. 2024

Date of Issue : 27 Aug. 2024

Ref : 2011167080602911001

End of Certificate

3 / 3

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.5

Head Office

35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9009

Office/Laboratory

668 Mu 2 Tambon Bangpoomai, Amphoe Muang Samutprakan,
Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtc@tistr.or.th Website : www.tistr.or.th

Office

196 Phahonyothin Road, Ladyao, Chatuchak,
Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827



SMART TECH CALIBRATION & SERVICES CO., LTD.

14/506 MOO 3, RANGSIT-NAKHON NAYOK ROAD, LAM PHAK KUT,
THANYABURI, PATHUM THANI 12110, THAILAND
Tel. +662-114-3148 Email : stcal.md@gmail.com Website : stc-cal.com



Certificate of Calibration

Certificate No. STCR-2401076-1

Work Order No. STCR-2401076

Page 1 of 3

Customer Name : TNP Environment Co., Ltd.
332/173 Vision Smart Life Village, Bang Rak Pattana Subdistrict,
Bang Bua Thong District, Nonthaburi Province 11110

Equipment Name : Sound Level Meter
Manufacturer : Pulsar
Model : 44
Serial Number : PN2351
Control Number : TNP-F-S22
Received Date : Jan 13, 2024
Calibration Date : Jan 15, 2024
Recommended Due Date : Jan 15, 2025
Calibration Method : Calibration Procedure No. CPE-04-01

Environmental Conditions
Ambient Temperature : $(25 \pm 2) ^\circ\text{C}$
Ambient Relative Humidity : $(50 \pm 15) \% \text{RH}$
Calibration Place : Permanent Calibration Laboratory

Condition as received : Normal
Calibration Result : See data attached

1. The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%.
2. The Unit Under Calibration (UUC) has been calibrated by using the working standard which is traceable to SI-Units. The calibration procedure documented is intended to implement the requirements of ISO/IEC 17025 : 2017
3. The working standard is indicated in page 2 of this certificate.
4. This report applies to the item calibrated and shall not be reproduced except in full, without written approval by Calibration Laboratory, Smart Tech Calibration & Services Co., Ltd.
5. This results of this report only to the items calibrated.

Date of Issue :

Approved by :

Calibrated by :



@smarttechcal

Calibration Report

Smart Tech Calibration & Services Co., Ltd.

Certificate No.: STCR-2401076-1

Page 2 of 3

Standards Equipment Used

<u>Equipment Name</u>	<u>Serial No.</u>	<u>Certificate No.</u>	<u>Due Date</u>	<u>Traceability to</u>
Sound Calibrator	N975186	5523631030478623	Nov 9, 2024	MP-TH

Traceability

This calibration is traceable to the International System of Unit via :

- MP-TH : Micro Precision Calibration Laboratory (Thailand) Co., Ltd.



Calibration Report

Smart Tech Calibration & Services Co., Ltd.

Certificate No.: STCR-2401076-1

Page 3 of 3

UUC Range : (20 to 140) dB

Resolution : 0.1 dB

Results of Calibration: [] Without adjustment [☒] With adjustment

Appearance and Function of Use Inspection : GOOD

Sound Level Calibration @ Frequency 1 kHz

Select : A

Response times	STD. Value	UUC. Reading		Correction	(±) Uncertainty
		Before Adjustment	After Adjustment		
FAST	94.09 dB	94.7 dB	94.1 dB	-0.01 dB	0.40 dB
	114.07 dB	114.7 dB	114.0 dB	0.07 dB	0.40 dB
SLOW	94.09 dB	94.7 dB	94.1 dB	-0.01 dB	0.40 dB
	114.07 dB	114.6 dB	114.0 dB	0.07 dB	0.40 dB

STD = Standard

UUC = Unit Under Calibration

- End of Certificate -



**SMART TECH CALIBRATION & SERVICES CO., LTD.**

14/506 MOO 3, RANGSIT-NAKHON NAYOK ROAD, LAM PHAK KUT,
THANYABURI, PATHUM THANI 12110, THAILAND

Tel. +662-114-3148 Email : stcal.md@gmail.com Website : stc-cal.com



Certificate of Calibration

Certificate No. STCR-2407092-1

Work Order No. STCR-2407092

Page 1 of 3

Customer Name : TNP Environment Co., Ltd.
332/173 Vision Smart Life Village, Bang Rak Pattana Subdistrict,
Bang Bua Thong District, Nonthaburi Province 11110

Equipment Name : Sound Level Meter
Manufacturer : SCARLET
Model : ST-25D
Serial Number : 10340945
Control Number : TNP-F-S25
Received Date : Jul 4, 2024
Calibration Date : Jul 5, 2024
Recommended Due Date : Jul 5, 2025
Calibration Method : Calibration Procedure No. CPE-04-01

Environmental Conditions

Ambient Temperature : $(25 \pm 2) ^\circ\text{C}$
Ambient Relative Humidity : $(50 \pm 15) \% \text{RH}$
Calibration Place : Permanent Calibration Laboratory

Condition as received : Normal

Calibration Result : See data attached

1. The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%.
2. The Unit Under Calibration (UUC) has been calibrated by using the working standard which is traceable to SI-Units. The calibration procedure documented is intended to implement the requirements of ISO/IEC 17025 : 2017
3. The working standard is indicated in page 2 of this certificate.
4. This report applies to the item calibrated and shall not be reproduced except in full, without written approval by Calibration Laboratory, Smart Tech Calibration & Services Co., Ltd.
5. This results of this report only to the items calibrated.

Date of Issue :

Calibrated by :

Approved by :



@smarttechcal

Calibration Report

Smart Tech Calibration & Services Co., Ltd.

Certificate No.: STCR-2407092-1

Page 2 of 3

Standards Equipment Used

<u>Equipment Name</u>	<u>Serial No.</u>	<u>Certificate No.</u>	<u>Due Date</u>	<u>Traceability to</u>
Sound Calibrator	N975185	5523631030478623	Nov 9, 2024	MP-TH

Traceability

This calibration is traceable to the International System of Unit via :

- MP-TH : Micro Precision Calibration Laboratory (Thailand) Co., Ltd.



Calibration Report

Smart Tech Calibration & Services Co., Ltd.

Certificate No.: STCR-2407092-1

Page 3 of 3

UUC Range : (30 to 130) dB

Resolution : 0.1 dB

Results of Calibration: [] Without adjustment [☒] With adjustment

Appearance and Function of Use Inspection : GOOD

Sound Level Calibration @ Frequency 1 kHz

Select : A

Response times	STD. Value	UUC. Reading		Correction	(±) Uncertainty
		Before Adjustment	After Adjustment		
FAST	94.09 dB	93.2 dB	94.1 dB	-0.01 dB	0.40 dB
	114.07 dB	113.1 dB	114.0 dB	0.07 dB	0.40 dB
SLOW	94.09 dB	93.2 dB	94.1 dB	-0.01 dB	0.40 dB
	114.07 dB	113.1 dB	113.9 dB	0.17 dB	0.40 dB

Sound Level Calibration @ Frequency 1 kHz

Select : C

Response times	STD. Value	UUC. Reading		Correction	(±) Uncertainty
		Before Adjustment	After Adjustment		
FAST	94.09 dB	93.2 dB	94.1 dB	-0.01 dB	0.40 dB
	114.07 dB	113.1 dB	114.0 dB	0.07 dB	0.40 dB
SLOW	94.09 dB	93.2 dB	94.1 dB	-0.01 dB	0.40 dB
	114.07 dB	113.2 dB	114.0 dB	0.07 dB	0.40 dB

STD = Standard

UUC = Unit Under Calibration

- End of Certificate -





CALIBRATION LABORATORY Co., LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



CERTIFICATE OF CALIBRATION

FOR

NOMENCLATURE : VIBRATION METER
MANUFACTURER : INSTANTEL
MODEL / TYPE : 721A2601/721A3301
SERIAL NO. : UM14102/UM14102
CLID. NO. : 252100393
JOB CONTROL NO. : 241101116709
CALIBRATION SERVICE : ☒ IN-LABORATORY ☐ ON-SITE


CUSTOMER : TNP ENVIRONMENT CO., LTD.
332/173 MOO 3 TAMBON BANG RAK PHATTANA,
AMPHOE BANG BUA THONG, NONTHABURI 11110

DATE OF RECEIVED : 01 November 2024

DATE OF ISSUED : 06 November 2024

The report of calibration shall not be reproduced except in full without approval of the Calibration Laboratory Co., Ltd.

Calibrated By :



Approved By :



06 November 2024

This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to the
International System of Units (SI)

Certificate No. Q24116709

F3-011-05/12-23

page 1 of 4



@clccalibration

REPORT OF CALIBRATION FOR

NOMENCLATURE : **VIBRATION METER**
MANUFACTURER : **INSTANTEL**
MODEL / TYPE : **721A2601/721A3301**
SERIAL NO. : **UM14102/UM14102**
DATE OF CALIBRATION : **04 November 2024**

ENVIRONMENT CONDITIONS :

Temperature : $(23 \pm 2) ^\circ\text{C}$

Relative Humidity : $(55 \pm 15) \% \text{RH}$

PROCEDURE USED :

This instrument was calibrated under procedure No. **CLC-CPEE-08** based on **ISO 16063-21** as calibration guideline.

The calibration was performed by using Digital Multimeter, Programmable Timer/Counter, Vibration Calibrator which maintained by the Calibration Laboratory Co., Ltd.

REFERENCE STANDARD USED :

1. Vibration Calibrator, The Modal Shop Model 9110D S/N. 11424.
2. Digital Multimeter, Hewlett Packard Model 34401A S/N. 3146A75935.
3. Programmable Timer/Counter, Philips Model PM6680B S/N. SM607101.

TRACEABILITY :

1. The measurements are traceable to International System of Units (SI), through National Institute of Metrology (Thailand) Certificate No. AV-0030-24, Due Date 19 July 2025.
2. The measurements are traceable to International System of Units (SI), through National Institute of Metrology (Thailand) Certificate No. EE-0130-23, Due Date 29 November 2024.
3. The measurements are traceable to International System of Units (SI), through Aeronautical Radio of Thailand Ltd. Certificate No. 07-0050/24, Due Date 13 May 2025.

UNCERTAINTY :

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor $k = 2,00$ which for a normal distribution corresponds to a coverage probability of approximately 95 %.

It has been evaluated according to the "Evaluation of the Uncertainty of Measurement in Calibration (EA-4/02 M:2022)"

Certificate No. Q24116709

F3-011-05/12-23

page 2 of 4





CLC
Accredited
ISO/IEC 17025

CALIBRATION LABORATORY Co., LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



CONDITION OF CALIBRATION ITEM : RECEIVED IN GOOD OPERATIONAL CONDITION

MEASUREMENT RESULTS : (X) without adjustment () adjustment

CALIBRATION DATA

1. VELOCITY RESULT

Test point		Mode	STD Reading	DUC Reading	Correction	Uncertainty
(mm/s)	(frequency)		(mm/s)	(mm/s)	(mm/s)	± (% of rdg.)
10	80 Hz	peak	10.000	10.097	-0.097	1.5
20	80 Hz		20.000	20.188	-0.188	1.5
30	80 Hz		30.000	30.256	-0.256	1.5
40	80 Hz		40.000	40.365	-0.365	1.5
50	80 Hz		50.000	50.421	-0.421	1.5

Note. The Scope of Accredited ANAB Certificate No. ACDM-2814 Version 012 Page 2 of 67

Certificate No. Q24116709

F3-011-05/12-23

page 3 of 4



@clccalibration

CALIBRATION DATA

*2. FREQUENCY RESULT

STD Applied (Hz)	DUC Reading (Hz)	Correction (Hz)	Uncertainty \pm (Hz)
50	50	0	0.6
80	79	+1	0.6
100	100	0	0.6

Note. * means Calibrations marked " Not ANAB Accredited " in this Certificate have been included for completeness.

This report is valid for the above stated instrument/s only.

End of Certificate

Certificate No. Q24116709

F3-011-05/12-23

page 4 of 4



@clccalibration



ID LINE : IEC17025



Certificate of Calibration

Certificate Number : SPR24050187-1

Page : 1 of 3

Customer : TNP ENVIRONMENT CO.,LTD.

332/173 Moo.3, Bang Rak Phatthana, Bang Bua Thong, Nonthaburi
11110

Equipment Name : Autoclave

Manufacturer : BIOBASE

Model : BKQ-Z50I

Serial Number : BKQ-Z50I23055014

ID. Number : TNP.LAB.56

Environmental Conditions

Ambient Temperature : $25^{\circ}\text{C} \pm 10^{\circ}\text{C}$

Relative Humidity : $60\% \pm 20\%$

Location of Calibration : On-Site

Calibration Procedure : SP-CPT-04-04

Received Date : 11 May 2024

Calibration Date : 16 May 2024

Recommend Due Date : 16 May 2025

Date of Issue : 17 May 2024

Method of Calibration

This certifies that the above instrument was calibrated in compliance with the calibration system requirement of ISO/IEC 17025:2017 in accordance with reference procedure. Standards used to perform this calibration are certified by to NIST or equivalent, National metrology institute, Natural physical constants, consensus standards. The result reported herein apply only to the calibration of the item described above as received. Our decision rule is to contact the customer if the item pass and fail calibration when the results include the uncertainties and the customer must determine if the results meets their needs.


The calibration certificate shall not be reproduced except in full, without written approval of SP Metrology System (Thailand).

Calibrated by :



Calibration Officer

Approved by :



Authorized Signatory



ID LINE : IEC17025



Calibration Report

Certificate Number : SPR24050187-1

Page : 2 of 3

Reference Standards

Equipment Name	Model	Serial No.	Certificate No.	Due. Date
Data Acquisition/Switch Unit	34970A	MY44074688	SPR24010142-25	11 Jan 2025

Traceability

This certification is traceable to the International System of Unit maintained at :
SP Metrology - SP Metrology system (Thailand) Co.Ltd.




ID LINE : IEC17025



Result of Calibration

Certificate Number : SPR24050187-1

Page : 3 of 3

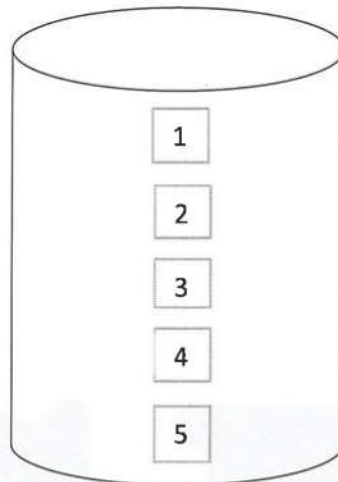

1. Temperature Accuracy in the Measurement Zone.

Unit : °C

UUC Setting	Measured Temperature (°C) @ Probe No.					Uncertainty (±)
	# 1	# 2	# 3	# 4	# 5	
115.0	115.1	115.0	115.1	115.0	115.1	0.26
121.0	121.1	121.0	121.0	121.1	121.1	0.26

2. Temperature Uniformity, Stability

Unit : °C

UUC Setting	UUC Reading	Temperature Stability	Temperature Uniformity
115.0	115.0	0.02	0.04
121.0	121.0	0.02	0.04

Note :

The result of calibration was found accurate as show on date and place of calibration only.
This Certificate is not certified for any commercial transaction.

Measurement Uncertainty

The reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor $k = 2.00$, providing a level of confidence approximately 95 %

- End of Certificate -



ID LINE : IEC17025



Certificate of Calibration

Certificate Number : SPR24050187-2

Page : 1 of 3

Customer : TNP ENVIRONMENT CO.,LTD.

332/173 Moo.3, Bang Rak Phatthana, Bang Bua Thong, Nonthaburi
11110

Equipment Name : pH Meter

Manufacturer : Eutech

Model : pH 700

Serial Number : 3178920

ID. Number : TNP.LAB.57

Environmental Conditions

Ambient Temperature : $25^{\circ}\text{C} \pm 10^{\circ}\text{C}$

Relative Humidity : $60\% \pm 20\%$

Location of Calibration : On-Site

Calibration Procedure : SP-CPC-04-01

Received Date : 11 May 2024

Calibration Date : 16 May 2024

Recommend Due Date : 16 May 2025

Date of Issue : 17 May 2024

Method of Calibration

This certifies that the above instrument was calibrated in compliance with the calibration system requirement of ISO/IEC 17025:2017 in accordance with reference procedure. Standards used to perform this calibration are certified by to NIST or equivalent, National metrology institute, Natural physical constants, consensus standards. The result reported herein apply only to the calibration of the item described above as received. Our decision rule is to contact the customer if the item pass and fail calibration when the results include the uncertainties and the customer must determine if the results meets their needs.


The calibration certificate shall not be reproduced except in full, without written approval of SP Metrology System (Thailand).

Calibrated by :



Calibration Officer

Approved by



Authorized Signatory



ID LINE : IEC17025



Calibration Report

Certificate Number : SPR24050187-2

Page : 2 of 3

Reference Standards

Equipment Name	Model	Serial No.	Certificate No.	Due. Date
Standard pH Solution	PH016.L5	Lot No.970880	61278486	25 Apr 2025
Standard pH Solution	PH107.L5	Lot No.970881	61281486	25 Apr 2025
Standard pH Solution	PH020.L5	Lot No.970882	61297722	25 Apr 2025

Traceability

This certification is traceable to the International System of Unit maintained at :
C.P.A. Chem - ANAB#AT-1836 (ISO/IEC 17025:2017) and ANAB#AR-1835 (ISO/IEC
17034:2016)



ID LINE : IEC17025



Result of Calibration

Certificate Number : SPR24050187-2

Page : 3 of 3

Range : 0 to 14 pH

Resolution : 0.01 pH

pH Measurement @ 25 °C

Unit : pH

Standard Solution	UUC Reading	Error	Uncertainty (±)
4.008	4.03	0.022	0.012
6.984	7.00	0.016	0.012
10.011	9.96	-0.051	0.013

Note :

The result of calibration was found accurate as show on date and place of calibration only.
This Certificate is not certified for any commercial transaction.

Measurement Uncertainty

The reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor $k = 2.00$, providing a level of confidence approximately 95%.

- End of Certificate -



ID LINE : IEC17025



Certificate of Calibration

Certificate Number : SPR24050187-3

Page : 1 of 3

Customer : TNP ENVIRONMENT CO.,LTD.

332/173 Moo.3, Bang Rak Phatthana, Bang Bua Thong, Nonthaburi
11110

Equipment Name : Water Bath

Manufacturer : Memmert

Model : WTB24

Serial Number : LD23.0297

ID. Number : TNP.LAB.58

Environmental Conditions

Ambient Temperature : $25^{\circ}\text{C} \pm 10^{\circ}\text{C}$

Relative Humidity : $60\% \pm 20\%$

Location of Calibration : On-Site

Calibration Procedure : SP-CPT-04-04

Received Date : 11 May 2024

Calibration Date : 16 May 2024

Recommend Due Date : 16 May 2025

Date of Issue : 17 May 2024

Method of Calibration

This certifies that the above instrument was calibrated in compliance with the calibration system requirement of ISO/IEC 17025:2017 in accordance with reference procedure. Standards used to perform this calibration are certified by to NIST or equivalent, National metrology institute, Natural physical constants, consensus standards. The result reported herein apply only to the calibration of the item described above as received. Our decision rule is to contact the customer if the item pass and fail calibration when the results include the uncertainties and the customer must determine if the results meets their needs.


The calibration certificate shall not be reproduced except in full, without written approval of SP Metrology System (Thailand).

Calibrated by :



Calibration Officer

Approved by :

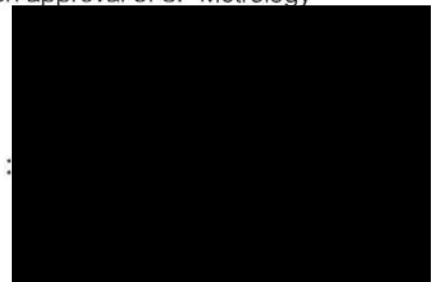

Authorized Signatory



ID LINE : IEC17025



Calibration Report

Certificate Number : SPR24050187-3

Page : 2 of 3

Reference Standards

Equipment Name	Model	Serial No.	Certificate No.	Due. Date
Data Acquisition/Switch Unit	34970A	MY44074688	SPR24010142-25	11 Jan 2025

Traceability

This certification is traceable to the International System of Unit maintained at :
SP Metrology - SP Metrology system (Thailand) Co.Ltd.




ID LINE : IEC17025



Result of Calibration

Certificate Number : SPR24050187-3

Page : 3 of 3

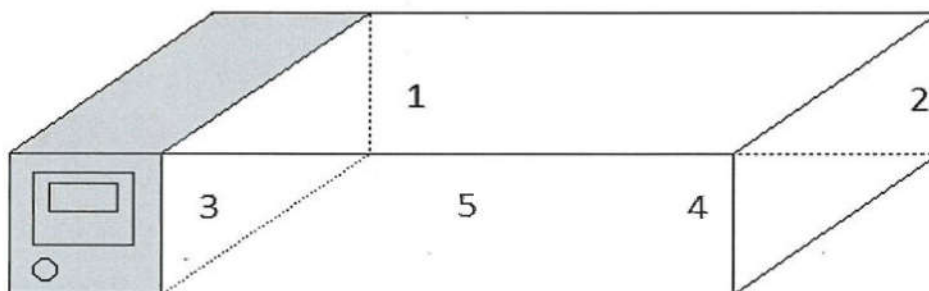

1. Temperature Accuracy in the Measurement Zone.

Unit : °C

UUC Setting	Measured Temperature (°C) @ Probe No.					Uncertainty (±)
	# 1	# 2	# 3	# 4	# 5	
44.5	44.54	44.44	44.50	44.50	44.47	0.19

2. Temperature Uniformity, Stability

Unit : °C

UUC Setting	UUC Reading	Temperature Stability	Temperature Uniformity
44.5	44.5	0.07	0.20

Note :

The result of calibration was found accurate as show on date and place of calibration only.
This Certificate is not certified for any commercial transaction.

Measurement Uncertainty

The reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor $k = 2.00$, providing a level of confidence approximately 95 %

- End of Certificate -



ID LINE : IEC17025



Certificate of Calibration

Certificate Number : SPR24050187-4

Page : 1 of 3

Customer : TNP ENVIRONMENT CO.,LTD.

332/173 Moo.3, Bang Rak Phatthana, Bang Bua Thong, Nonthaburi
11110

Equipment Name : Incubator

Manufacturer : BIOBASE

Model : BJPX-M100B

Serial Number : BJPXM1002301016

ID. Number : TNP.LAB.59

Environmental Conditions

Ambient Temperature : $25^{\circ}\text{C} \pm 10^{\circ}\text{C}$

Relative Humidity : $60\% \pm 20\%$

Location of Calibration : On-Site

Calibration Procedure : SP-CPT-04-01

Received Date : 11 May 2024

Calibration Date : 16 May 2024

Recommend Due Date : 16 May 2025

Date of Issue : 17 May 2024

Method of Calibration

This certifies that the above instrument was calibrated in compliance with the calibration system requirement of ISO/IEC 17025:2017 in accordance with reference procedure. Standards used to perform this calibration are certified by to NIST or equivalent, National metrology institute, Natural physical constants, consensus standards. The result reported herein apply only to the calibration of the item described above as received. Our decision rule is to contact the customer if the item pass and fail calibration when the results include the uncertainties and the customer must determine if the results meets their needs.


The calibration certificate shall not be reproduced except in full, without written approval of SP Metrology System (Thailand).

Calibrated by :



Calibration Officer

Approved by :

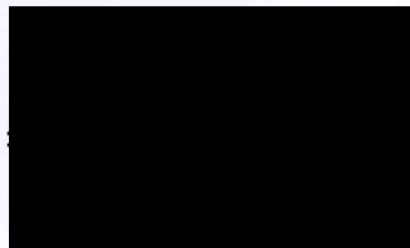

Authorized Signatory



ID LINE : IEC17025



Calibration Report

Certificate Number : SPR24050187-4

Page : 2 of 3

Reference Standards

Equipment Name	Model	Serial No.	Certificate No.	Due. Date
Data Acquisition/Switch Unit	34970A	MY44074688	SPR24010142-25	11 Jan 2025

Traceability

This certification is traceable to the International System of Unit maintained at :
SP Metrology - SP Metrology system (Thailand) Co.Ltd.




ID LINE : IEC17025



Result of Calibration

Certificate Number : SPR24050187-4

Page : 3 of 3

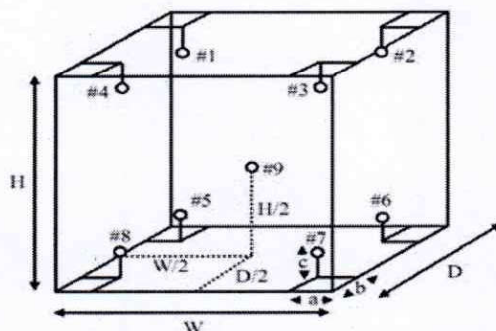

Temperature Accuracy in the Measurement Zone.

Unit : °C

UUC Setting	Measured Temperature (°C) @ Probe No. (Probe No. 9 is REF.)									Uncertainty (±)
	# 1	# 2	# 3	# 4	# 5	# 6	# 7	# 8	# 9	
35.0	35.20	35.17	35.26	35.22	35.28	35.18	35.24	35.22	35.28	0.19
37.0	37.16	37.24	37.24	37.20	37.23	37.27	37.19	37.23	37.28	0.19
41.5	41.68	41.72	41.77	41.72	41.67	41.74	41.74	41.75	41.79	0.19
42.0	42.22	42.25	42.18	42.28	42.30	42.32	42.27	42.31	42.33	0.19

Temperature Uniformity, Stability, Overall Variation

Unit : °C

UUC Setting	UUC Reading	Temperature Stability	Temperature Uniformity	Overall Variation
35.0	35.0	0.09	0.30	0.30
37.0	37.0	0.11	0.32	0.33
41.5	41.5	0.09	0.26	0.28
42.0	42.0	0.10	0.31	0.36

Note :

The result of calibration was found accurate as show on date and place of calibration only.
This Certificate is not certified for any commercial transaction.

Measurement Uncertainty

The reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor $k = 2$, providing a level of confidence approximately 95 %

- End of Certificate -

Certificate No. T/O 670044

Date of issue : 15-Mar-2024

Equipment Description : Incubator

Equipment Model : SMART i250-DS

Equipment Serial No. : 0410-0121-0003

I.D. No. or Control No. : -

Manufacturer : Entech Industrial Solution Co.,Ltd.

Customer Name : TNP ENVIRONMENT.CO.,LTD

Customer Address : 332/173 Bang Rak Phatthana Subdistrict, Bang Bua Thong District,
Nonthaburi 11110

Total pages of certificate : 2 pages

Instrument Receiving Date : 14-Mar-2024

Receiving No. : O-240062

Environmental Conditions : All of the measurement were carried out in the working area
Temperature : (25 ± 15) °C
Humidity : (55 ± 30) % RH
Voltage : (220 ± 22) VAC

Calibration Place : (TNP Lab) 332/173 Bang Rak Phatthana Subdistrict,Bang Bua Thong District,
Nonthaburi 11110 Thailand

Calibration Procedure No. : This instrument was calibrated by comparison of reference radiation source standard
according to calibration work instruction no WI-CL-18-C

The calibration certificate expended uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k , which for a normal distribution corresponds to a coverage probability of approximately 95%

The standard uncertainty of measurement has been determined in accordance with M 3003



The expression uncertainty and confidence in measurement.

This certificate is applied only to item under test environmental condition.

This calibration certificate may not be reproduced other than in full except with the permission of the issuing laboratory. Calibration certificates without signature and seal are not valid and The results relate only to the items tested/calibrated .

This calibration certificate documents are traceability to national standards, which realize the unit of measurement according to the International system of units (SI).

Date of Calibration : 14-Mar-2024



Certificate No. : T/O 670044


The Reference Standard Instrument :-

Instrument	Model	Serial No.	Cert No.	Due date
1) Data logger with RTD Probe	Agilent 34972A	MY49017365	PSL-T 0484-3/67	19-Feb-2025

Measured room conditions

Temperature :	Minimum: 23.6 °C	Maximum: 24.2 °C
Humidity :	Minimum: 48.5 %RH	Maximum: 56.9 %RH
Voltage :	Minimum: 220.1 VAC	Maximum: 223.4 VAC
Fresh Air Setting:	off	

Sensor Position :

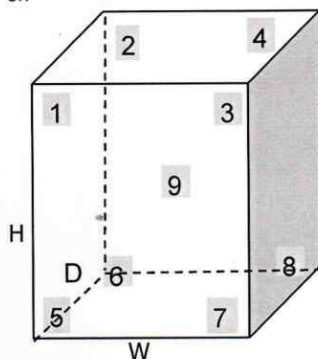

Working Space of chamber :

(Inside Dimensions) W x D x H : 500 mm x 480 mm x 1100 mm

Sensor Installation Details :

- Sensor Number 1 to 8 installed approximately 50 mm From each wall.
- Sensor Number 9 installed approximately geometric of the chamber.

Results : The measurement results of the calibration were reported in the table below.

(*) Without adjustment

() After adjustment

UUC*	UUC*	Temperature Reading of Standard Sensor								
Setting	Reading	Sensor Position								
(°C)	(°C)	1	2	3	4	5	6	7	8	9
20.0	20.0	20.50	19.56	20.31	20.34	20.41	20.28	20.18	20.21	20.30

UUC*	UUC*	Temperature	Temperature	Overall	Uncertainty	Coverage
Setting	Reading	Uniformity	Stability	Variation	of Measurement	Factor
(°C)	(°C)	(°C)	(± °C)	(°C)	(± °C)	K
20.0	20.0	0.88	0.37	1.33	0.51	2

UUC* = Unit Under Calibration

Remark :-

- Temperature reading of Standard Sensors shown in the table were taken from the average of Standard reading at each position.
- Temperature Uniformity was calculated from the difference between the maximum and minimum of actual temperature reading from all reference sensors at the same time.
- Temperature Stability was calculated from the maximum stability of nine positions, and formula of Stability is [(Maximum Temperature Value - Minimum Temperature Value) / 2]
- Overall Variation was calculated from the difference between the maximum and minimum measured temperature throughout observation time.

End of Report



THAI CALIBRATION SERVICES CO., LTD.

19/8 Moo 9 Soi Raiking 30 Puttamonthon 5 Rd., Sampran, Nakornpatom 73210

Tel. 0-3439-7682-5 Fax: 0-3439-7687

www.thaical.com E-mail : sale@thaicalibration.com, lab@thaicalibration.com



CALIBRATION CERTIFICATE

Certificate No.S2406450S

page 1 of 2

Customer : TNP ENVIRONMENT CO., LTD.
332/173 Moo 3 Tambon Bang Rak Phatthana,
Amphoe Bang Bua Thong, Nonthaburi 11110

Equipment : Non-automatic weighing instrument (Electronic instrument)

Manufacturer : Sartorius **Order No. :** 67S2626-1

Model : SECURA224-1S **Ambient temperature :** $(27.3 \pm 5.0) ^\circ\text{C}$

Accuracy class : - **Relative humidity :** $(33.0 \pm 10.0) \%$

Capacity : 220 g **Received date :** 17-Jun-2024

Resolution : 0.0001 g **Date of calibration :** 17-Jun-2024

Serial No. : 0041305301 **Date of issue :** 19-Jun-2024

ID No. : TNP.LAB.31 **Condition of the balance :** Good working conditions

Place of calibration : ห้อง LAB

Calibration method

This instrument was calibrated according to the EURAMET Calibration Guide No. 18.

Condition of reference standard weight

Instrument	Nominal value	Serial No.	Certificate No.	Due-date	Density (kg/m ³)
1 Standard weight set	1 mg to 2 kg	15885+15849	M2310001S	7-Oct-2024	7950

Traceability of the reference standard weight


This certificate is traceable to SI unit through Mass Calibration Laboratory Thai Calibration Services Co., Ltd., NSC-ONSC accredited no. Calibration 0189.

Calibrated By :



Technician

Approved Signato

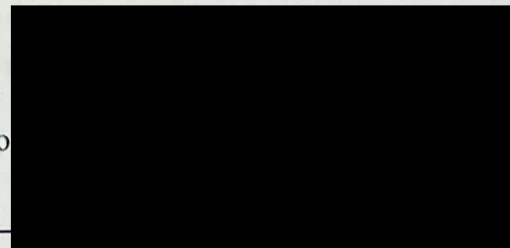

This calibration certificate may not be reproduced other than in full,
except with the prior written approval of the head of TCS calibration laboratory.



THAI CALIBRATION SERVICES CO., LTD.

19/8 Moo 9 Soi Raking 30 Puttamonthon 5 Rd., Sampran, Nakornpatom 73210

Tel. 0-3439-7682-5 Fax: 0-3439-7687

www.thaical.com E-mail : sale@thaicalibration.com, lab@thaicalibration.com



NSC-TISI-TIS 17025
CALIBRATION 0189

CALIBRATION CERTIFICATE

Certificate No.S2406450S


page 2 of 2

The repeatability of indication

Nominal Value (g)	Standard Deviation of reading (g)	Maximum difference between successive reading (g)	n
200	0.00000	0.0000	5

The effect of eccentric application of a load on the indication (test load : 100 g)

Position	Balance Reading (g)
Point 1	100.0000
Point 2	99.9999
Point 3	100.0000
Point 4	100.0000
Point 5	100.0000
Eccentric Value	0.0001



The error of indication

Nominal Value (g)	Value of Reference Standard Weight (g)	Balance Reading (g)	Correction (g)	Uncertainty (±) (g)	k
Unload	0.0000	0.0000	0.0000	0.000082	2.00
0.1	0.1000	0.1000	0.0000	0.000083	2.00
0.5	0.5000	0.5000	0.0000	0.000084	2.00
1	1.0000	1.0000	0.0000	0.000085	2.00
5	5.0000	5.0001	-0.0001	0.000089	2.00
10	10.0000	10.0000	0.0000	0.000093	2.00
20	20.0000	20.0000	0.0000	0.00010	2.00
50	50.0000	50.0000	0.0000	0.00012	2.00
100	99.9999	100.0000	-0.0001	0.00015	2.00
200	199.9999	199.9999	0.0000	0.00026	2.00

Remark : Adjustment, External weight nominal value 200 g, Standard weight of Lab

Uncertainty of measurement

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor (k), which for a normal distribution corresponds to a coverage probability of approximately 95% (confidence level).

This report will certify of the calibrated equipment only.

--End--

Certificate no: H/T 670338

Date of issue : 21-Mar-24

Instrument description	:	Thermo-Hygrometer
Instrument model	:	Extech 445815
Instrument serial no.	:	PONPE5899554
ID no. or control no.	:	TNP.LAB.21
Manufacturer	:	Extech Instruments
Probe description	:	-
Probe model	:	-
Probe serial	:	-
Customer name	:	TNP ENVIRONMENT CO.,LTD.
Customer address	:	332/173 Moo 3 Tambon Bang Rak Phatthana, Amphoe Bang Bua Thong, Nonthaburi 11110
 Total pages of certificate	:	 2 Pages
Receiving no.	:	L-241004-1
Receiving date.	:	08-Mar-24
Parameter of calibration	:	Temperature Calibration
Condition of UUC.	:	Used
Ambient condition	:	All of the Measurement were carried out the stabilized laboratory
		Temperature : 23 ± 5 °C
		Humidity : 55 ± 15 %RH
Calibration place	:	17/121 Soi Ngamwongwan 47 Yaek 48, Toongsonghong, Laksi, Bangkok 10210
 Calibration procedure no.	:	 This instrument was calibrated by comparison of indication with the Standard Thermo- hygrometer according to calibration Work Instruction no .WI-CL-11-C


The calibration certificate expanded uncertainty of measurement is stated as the standard uncertainty of measurent Multiplied by coverage factor $k=2$, which for a normal distribution corresponds to a coverage probability of approximately 95%.

This certificate is applied only to item under test Environmental condition.


This Calibration Certificate may not be reporduced other than in full except with the permission of the issuing laboratory. Calibration certificates without signature and seal not valid.

This calibration certificate documents are tracebility to national standards, which realize measurement according to the International System of Units (SI).

Date of calibration : 20-Mar-24



Calibration Technician



Technical Manager

Certificate no: H/T 670338

Standard refereces

Standard	Reference No.	Vendor	Due Date
ARALAB 300ECP,Fitoclima	S2023070040-001	MIT	07-Jul-24
Thermo HygroPalm HP 23-A	SG-H-00579/66	Success Gateway	16-Aug-24

Measured room conditions

Temperature : 22.1 °C

Humidity : 55.9 %RH

Pressure : 1019.3 mbar

Calibration results (Without Adjustment)

Reference temperature : - °C

Parameter of standard	Standard values	Mean of UUC.	Error	Uncertainty (±)
Temperature (°C)	19.97	20.1	0.13	0.50
Temperature (°C)	25.02	25.2	0.18	0.50
Temperature (°C)	29.99	30.2	0.21	0.50

Remark : -

End of Report



THAI CALIBRATION SERVICES CO., LTD.

19/8 Moo 9 Soi Raiking 30 Puttamonton 5 Rd., Sampran, Nakornpatom 73210

Tel. 0-3439-7682-5 Fax: 0-3439-7687

www.thaical.com E-mail : sale@thaicalibration.com, lab@thaicalibration.com



CALIBRATION CERTIFICATE

Certificate No.S2406451S

page 1 of 2

Customer : TNP ENVIRONMENT CO., LTD.
332/173 Moo 3 Tambon Bang Rak Phatthana,
Amphoe Bang Bua Thong, Nonthaburi 11110

Equipment : Non-automatic weighing instrument (Electronic instrument)

Manufacturer : Shimadzu **Order No. :** 67S2626-2

Model : AP225WD **Ambient temperature :** $(27.2 \pm 5.0) ^\circ\text{C}$

Accuracy class : - **Relative humidity :** $(34.0 \pm 10.0) \%$

Capacity : 102 g / 220 g **Received date :** 17-Jun-2024

Resolution : 0.00001 g / 0.0001 g **Date of calibration :** 17-Jun-2024

Serial No. : D316301848 **Date of issue :** 19-Jun-2024

ID No. : TNP.LAB.30 **Condition of the balance :** Good working conditions

Place of calibration : ห้อง LAB

Calibration method

This instrument was calibrated according to the EURAMET Calibration Guide No. 18.

Condition of reference standard weight

Instrument	Nominal value	Serial No.	Certificate No.	Due-date	Density (kg/m ³)
1 Standard weight set	1 mg to 2 kg	15885+15849	M2310001S	7-Oct-2024	7950

Traceability of the reference standard weight


This certificate is traceable to SI unit through Mass Calibration Laboratory Thai Calibration Services Co., Ltd., NSC-ONSC accredited no. Calibration 0189.

Calibrated By :



Technician

Approved Signatory :



This calibration certificate may not be reproduced other than in full,
except with the prior written approval of the head of TCS calibration laboratory.



THAI CALIBRATION SERVICES CO., LTD.

19/8 Moo 9 Soi Raiking 30 Puttamonthon 5 Rd., Sampran, Nakornpatom 73210

Tel. 0-3439-7682-5 Fax: 0-3439-7687

www.thaical.com E-mail : sale@thaicalibration.com, lab@thaicalibration.com



CALIBRATION CERTIFICATE

Certificate No.S2406451S


page 2 of 2

The repeatability of indication

Nominal Value (g)	Standard Deviation of reading (g)	Maximum difference between successive reading (g)	n
100	0.000009	0.00002	5
200	0.00005	0.0001	5

The effect of eccentric application of a load on the indication (test load : 100 g)

Position	Balance Reading (g)
Point 1	100.00000
Point 2	100.00002
Point 3	100.00000
Point 4	99.99994
Point 5	99.99995
Eccentric Value	0.00006



The error of indication

Nominal Value (g)	Value of Reference Standard Weight (g)	Balance Reading (g)	Correction (g)	Uncertainty (±) (g)	k
Unload	0.00000	0.00000	0.00000	0.000027	2.65
0.1	0.10000	0.10003	-0.00003	0.000026	2.28
0.5	0.50000	0.50003	-0.00003	0.000029	2.15
1	1.00000	1.00004	-0.00004	0.000031	2.10
5	4.99998	5.00001	-0.00003	0.000041	2.03
10	9.99999	10.00002	-0.00003	0.000047	2.00
20	20.00000	19.99998	+0.00002	0.000060	2.00
50	50.00001	50.00003	-0.00002	0.000074	2.00
100	99.99995	100.00000	-0.00005	0.00012	2.00
200	199.9999	200.0000	-0.0001	0.00026	2.00

Remark : Adjustment, External weight nominal value 100 g, Standard weight of Lab

Uncertainty of measurement

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor (k), which for a normal distribution corresponds to a coverage probability of approximately 95% (confidence level).

This report will certify of the calibrated equipment only.

--End--



THAI CALIBRATION SERVICES CO., LTD.

19/8 Moo 9 Soi Raiking 30 Puttamonthon 5 Rd., Sampran, Nakornpatom 73210
Tel. 0-3439-7682-5 Fax: 0-3439-7687

www.thaical.com E-mail : sale@thaicalibration.com, lab@thaicalibration.com



CALIBRATION CERTIFICATE

Certificate No.S2406450S

page 1 of 2

Customer : TNP ENVIRONMENT CO., LTD.
332/173 Moo 3 Tambon Bang Rak Phatthana,
Amphoe Bang Bua Thong, Nonthaburi 11110

Equipment : Non-automatic weighing instrument (Electronic instrument)

Manufacturer : Sartorius **Order No. :** 67S2626-1

Model : SECURA224-1S **Ambient temperature :** $(27.3 \pm 5.0) ^\circ\text{C}$

Accuracy class : - **Relative humidity :** $(33.0 \pm 10.0) \%$

Capacity : 220 g **Received date :** 17-Jun-2024

Resolution : 0.0001 g **Date of calibration :** 17-Jun-2024

Serial No. : 0041305301 **Date of issue :** 19-Jun-2024

ID No. : TNP.LAB.31 **Condition of the balance :** Good working conditions

Place of calibration : ห้อง LAB

Calibration method

This instrument was calibrated according to the EURAMET Calibration Guide No. 18.


Condition of reference standard weight

<u>Instrument</u>	<u>Nominal value</u>	<u>Serial No.</u>	<u>Certificate No.</u>	<u>Due-date</u>	<u>Density (kg/m³)</u>
1 Standard weight set	1 mg to 2 kg	15885+15849	M2310001S	7-Oct-2024	7950


Traceability of the reference standard weight

This certificate is traceable to SI unit through Mass Calibration Laboratory Thai Calibration Services Co., Ltd., NSC-ONSC accredited no. Calibration 0189.

Calibrated By



Approved Signatory :

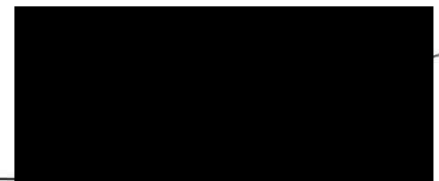

This calibration certificate may not be reproduced other than in full,
except with the prior written approval of the head of TCS calibration laboratory.



THAI CALIBRATION SERVICES CO., LTD.

19/8 Moo 9 Soi Raiking 30 Puttamonthon 5 Rd., Sampran, Nakornpatom 73210

Tel. 0-3439-7682-5 Fax: 0-3439-7687

www.thaical.com E-mail : sale@thaicalibration.com, lab@thaicalibration.com



NSC-TISI-TIS 17025
CALIBRATION 0189

CALIBRATION CERTIFICATE

Certificate No.S2406450S


page 2 of 2

The repeatability of indication

Nominal Value (g)	Standard Deviation of reading (g)	Maximum difference between successive reading (g)	n
200	0.00000	0.0000	5

The effect of eccentric application of a load on the indication (test load : 100 g)

Position	Balance Reading (g)
Point 1	100.0000
Point 2	99.9999
Point 3	100.0000
Point 4	100.0000
Point 5	100.0000
Eccentric Value	0.0001



The error of indication

Nominal Value (g)	Value of Reference Standard Weight (g)	Balance Reading (g)	Correction (g)	Uncertainty (±) (g)	k
Unload	0.0000	0.0000	0.0000	0.000082	2.00
0.1	0.1000	0.1000	0.0000	0.000083	2.00
0.5	0.5000	0.5000	0.0000	0.000084	2.00
1	1.0000	1.0000	0.0000	0.000085	2.00
5	5.0000	5.0001	-0.0001	0.000089	2.00
10	10.0000	10.0000	0.0000	0.000093	2.00
20	20.0000	20.0000	0.0000	0.00010	2.00
50	50.0000	50.0000	0.0000	0.00012	2.00
100	99.9999	100.0000	-0.0001	0.00015	2.00
200	199.9999	199.9999	0.0000	0.00026	2.00

Remark : Adjustment, External weight nominal value 200 g, Standard weight of Lab

Uncertainty of measurement

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor (k), which for a normal distribution corresponds to a coverage probability of approximately 95% (confidence level).

This report will certify of the calibrated equipment only.

--End--

CERT.No.: HS-V032E

Harikul Science Co.,Ltd.

694 Soi Ratchadanivet 24, Pracharatbamphen,
Samsaennok, Huaikhwang, Bangkok 10310

Tel: 0-2274-2456 Fax: 0-2274-2443

Email: info@harikul.com www.harikul.com

Certificate of Calibration

Calibration Date : 30 May 24

Submitted by : TNP ENVIRONMENT COMPANY LIMITED.

332/173 Moo. 3, Tambon Bang Rak Phatthana,

Amphoe Bang Bua Thong, Nonthaburi 11110

Avg Room Temp : 20 °C

Avg Water Temp : 20 °C

Air Pressure : 757.00 mmH

Salinity : 0 ppt

Model : YSI 4010-2W

S/N : 22051520

Probe : YSI 4100 BOD

S/N : 22C102711

ID NO. :

Air Temp ref : S/N. F8065C26

Barometric ref : S/N. F8065C26

Water Temp ref : S/N. 11431

Technician : Kittipong M.

Calibration Details

Calibration Point	100% air sat. (@20 °C, DO = 9.09 mg/l)	(status)	(status)
Measurement 1 (mg/l)	9.06	(PASS)	-
Measurement 2 (mg/l)	9.05	(PASS)	-
Measurement 3 (mg/l)	9.04	(PASS)	-
Measurement 4 (mg/l)	9.04	(PASS)	-
Measurement 5 (mg/l)	9.03	(PASS)	-
Measurement 6 (mg/l)	9.03	(PASS)	-
Measurement 7 (mg/l)	9.03	(PASS)	-
Measurement 8 (mg/l)	9.02	(PASS)	-
Measurement 9 (mg/l)	9.02	(PASS)	-
Measurement 10 (mg/l)	9.02	(PASS)	-



Mean Measurement	9.03	mg/l	-	-
Inaccuracy	0.06	mg/l	-	-

Overall Status (PASS)

Manufacturer Specification

Accuracy = +/- 0.2 mg/l

- 1) This certificate is issued based on the result that are found as shown on date and place of test only.
- 2) The calibration procedure followed in accordance with Harikul Science Co., Ltd.
- 3) This result shall not be used for advertising purpose.



CERT.No.: HS-V022D

Harikul Science Co.,Ltd.

694 Soi Ratchadanivet 24, Pracharatbamphen,
Samsaennok, Huaikhwang, Bangkok 10310

Tel: 0-2274-2456 Fax: 0-2274-2443

Email: info@harikul.com www.harikul.com

Certificate of Calibration

Calibration Date : 10 Apr 24

Submitted by : TNP ENVIRONMENT COMPANY LIMITED
332/173 Moo.3, Tambon Bang Rak Phatthana,
Amphoe Bang Bua Thong, Nonthaburi 11110

Model : HI 5421
S/N : 07210004101
Probe : HI 76408W
S/N : KC1N32W9P
ID NO. :
Air Temp ref : S/N. F8065C26
Barometric ref : S/N. F8065C26
Water Temp ref : S/N. 11430

Technician : Kittipong M.

Calibration Details

Calibration Point	100% air sat. (@20 °C, DO = 9.08 mg/l)	(status)	(status)
Measurement 1 (mg/l)	9.08	(PASS)	-
Measurement 2 (mg/l)	9.07	(PASS)	-
Measurement 3 (mg/l)	9.07	(PASS)	-
Measurement 4 (mg/l)	9.07	(PASS)	-
Measurement 5 (mg/l)	9.07	(PASS)	-
Measurement 6 (mg/l)	9.07	(PASS)	-
Measurement 7 (mg/l)	9.07	(PASS)	-
Measurement 8 (mg/l)	9.07	(PASS)	-
Measurement 9 (mg/l)	9.07	(PASS)	-
Measurement 10 (mg/l)	9.07	(PASS)	-
Mean Measurement	9.07	mg/l	-
Inaccuracy	0.01	mg/l	-

Overall Status (PASS)

Manufacturer Specification

Accuracy = +/- 0.15 mg/l

- 1) This certificate is issued based on the result that are found as shown on date and place of test only.
- 2) The calibration procedure followed in accordance with Harikul Science Co., Ltd.
- 3) This result shall not be used for advertising purpose.

Verification COD Reactor

Equipment Name Dri-Block Heater-Digital
 Serial No. 000827-A
 Reference Standard Thermocouple Type K
 Calibration Date 10/03/2023

Temperature Ver 150±2 °C
 Model DB 200/3
 Certificate No. 21/4272
 Next Cal. Date 10/03/2024

Left													
Hole 1				Hole 2				Hole 3					
NO.	Result			NO.	Result			NO.	Result				
	temp. °C	Corr.	temp+Corr.		temp. °C	Corr.	temp+Corr.		temp. °C	Corr.	temp+Corr.		
1	151.1	-0.36	150.7	1	150.6	-0.36	150.2	1	151.4	-0.36	151.0		
2	150.8	-0.36	150.4	2	151.7	-0.36	151.3	2	151.3	-0.36	150.9		
3	151.2	-0.36	150.8	3	151.1	-0.36	150.7	3	151.7	-0.36	151.3		
			Mean	150.67				Mean	150.77			Mean	151.11
			SD	0.208				SD	0.551			SD	0.208
			%RSD	0.138				%RSD	0.365			%RSD	0.138

Hole 4				Hole 5				Hole 6					
NO.	Result			NO.	Result			NO.	Result				
	temp. °C	Corr.	temp+Corr.		temp. °C	Corr.	temp+Corr.		temp. °C	Corr.	temp+Corr.		
1	151.7	-0.36	151.3	1	150.5	-0.36	150.1	1	151.5	-0.36	151.1		
2	151.6	-0.36	151.2	2	151.3	-0.36	150.9	2	151.4	-0.36	151.0		
3	151.5	-0.36	151.1	3	150.6	-0.36	150.2	3	150.5	-0.36	150.1		
			Mean	151.24				Mean	150.44			Mean	150.77
			SD	0.100				SD	0.436			SD	0.551
			%RSD	0.066				%RSD	0.290			%RSD	0.365

Hole 7				Hole 8				Hole 9					
NO.	Result			NO.	Result			NO.	Result				
	temp. °C	Corr.	temp+Corr.		temp. °C	Corr.	temp+Corr.		temp. °C	Corr.	temp+Corr.		
1	151.3	-0.36	150.9	1	151.7	-0.36	151.3	1	150.5	-0.36	150.1		
2	151.0	-0.36	150.6	2	150.5	-0.36	150.1	2	151.2	-0.36	150.8		
3	151.3	-0.36	150.9	3	151.4	-0.36	151.0	3	150.8	-0.36	150.4		
			Mean	150.84				Mean	150.84			Mean	150.47
			SD	0.173				SD	0.624			SD	0.351
			%RSD	0.115				%RSD	0.414			%RSD	0.233

Hole 10				Hole 11				Hole 12					
NO.	Result			NO.	Result			NO.	Result				
	temp. °C	Corr.	temp+Corr.		temp. °C	Corr.	temp+Corr.		temp. °C	Corr.	temp+Corr.		
1	151.6	-0.36	151.2	1	151.5	-0.36	151.1	1	150.7	-0.36	150.3		
2	151.6	-0.36	151.2	2	151.2	-0.36	150.8	2	151.6	-0.36	151.2		
3	150.8	-0.36	150.4	3	151.5	-0.36	151.1	3	151.2	-0.36	150.8		
			Mean	150.97				Mean	151.04			Mean	150.81
			SD	0.462				SD	0.173			SD	0.451
			%RSD	0.306				%RSD	0.115			%RSD	0.299

Verified By

Approved By

Confidential - Not to be photocopied except by permission of the Laboratory Quality Manager or nominee.

Verification COD Reactor

Equipment Name	Dri-Block Heater Digital	Temperature Ver	150±2 °C
Serial No.	000827-A	Model	DB 200/3
Reference Standard	Thermocouple Type K	Certificate No.	21/4272
Calibration Date	10/03/2023	Next Cal. Date	10/03/2024

Middle

Hole 1				Hole 2				Hole 3			
NO.	Result			NO.	Result			NO.	Result		
	temp. °C	Corr.	temp+Corr.		temp. °C	Corr.	temp+Corr.		temp. °C	Corr.	temp+Corr.
1	151.2	-0.36	150.8	1	150.7	-0.36	150.3	1	151.1	-0.36	150.7
2	151.5	-0.36	151.1	2	151.7	-0.36	151.3	2	151.6	-0.36	151.2
3	151.6	-0.36	151.2	3	150.8	-0.36	150.4	3	150.9	-0.36	150.5
		Mean	151.07			Mean	150.71			Mean	150.84
		SD	0.208			SD	0.551			SD	0.361
		%RSD	0.138			%RSD	0.365			%RSD	0.239

Hole 4				Hole 5				Hole 6			
NO.	Result			NO.	Result			NO.	Result		
	temp. °C	Corr.	temp+Corr.		temp. °C	Corr.	temp+Corr.		temp. °C	Corr.	temp+Corr.
1	151.5	-0.36	151.1	1	151.6	-0.36	151.2	1	150.5	-0.36	150.1
2	150.7	-0.36	150.3	2	151.2	-0.36	150.8	2	150.6	-0.36	150.2
3	151.6	-0.36	151.2	3	151.2	-0.36	150.8	3	151.2	-0.36	150.8
		Mean	150.91			Mean	150.97			Mean	150.41
		SD	0.493			SD	0.231			SD	0.379
		%RSD	0.327			%RSD	0.153			%RSD	0.252

Hole 7				Hole 8				Hole 9			
NO.	Result			NO.	Result			NO.	Result		
	temp. °C	Corr.	temp+Corr.		temp. °C	Corr.	temp+Corr.		temp. °C	Corr.	temp+Corr.
1	151.5	-0.36	151.1	1	151.5	-0.36	151.1	1	151.2	-0.36	150.8
2	150.5	-0.36	150.1	2	151.7	-0.36	151.3	2	150.9	-0.36	150.5
3	150.8	-0.36	150.4	3	151.1	-0.36	150.7	3	151.4	-0.36	151.0
		Mean	150.57			Mean	151.07			Mean	150.81
		SD	0.513			SD	0.306			SD	0.252
		%RSD	0.341			%RSD	0.202			%RSD	0.167

Hole 10				Hole 11				Hole 12			
NO.	Result			NO.	Result			NO.	Result		
	temp. °C	Corr.	temp+Corr.		temp. °C	Corr.	temp+Corr.		temp. °C	Corr.	temp+Corr.
1	151	-0.36	150.6	1	151.5	-0.36	151.1	1	151.2	-0.36	150.8
2	150.6	-0.36	150.2	2	150.6	-0.36	150.2	2	150.5	-0.36	150.1
3	151.5	-0.36	151.1	3	151.0	-0.36	150.6	3	151.1	-0.36	150.7
		Mean	150.67			Mean	150.67			Mean	150.57
		SD	0.451			SD	0.451			SD	0.379
		%RSD	0.299			%RSD	0.299			%RSD	0.251

Verified By

Approved By

Confidential - Not to be photocopied except by permission of the Laboratory Quality Manager or nominee.

Verification COD Reactor

Equipment Name Dri-Block Heater Digital
 Serial No. 000827/A
 Reference Standard Thermocouple Type K
 Calibration Date 10/03/2023

Temperature Ver 150±2 °C
 Model DB 200/3
 Certificate No. 21/4272
 Next Cal. Date 10/03/2024

Right

Hole 1				Hole 2				Hole 3			
NO.	Result			NO.	Result			NO.	Result		
	temp. °C	Corr.	temp+Corr.		temp. °C	Corr.	temp+Corr.		temp. °C	Corr.	temp+Corr.
1	149.9	-0.36	149.5	1	150.3	-0.36	149.9	1	151.0	-0.36	150.6
2	151.1	-0.36	150.7	2	151.0	-0.36	150.6	2	151.0	-0.36	150.6
3	150.9	-0.36	150.5	3	149.9	-0.36	149.5	3	150.4	-0.36	150.0
		Mean	150.27			Mean	150.04			Mean	150.44
		SD	0.643			SD	0.557			SD	0.346
		%RSD	0.428			%RSD	0.371			%RSD	0.230

Hole 4				Hole 5				Hole 6			
NO.	Result			NO.	Result			NO.	Result		
	temp. °C	Corr.	temp+Corr.		temp. °C	Corr.	temp+Corr.		temp. °C	Corr.	temp+Corr.
1	150.8	-0.36	150.4	1	150.0	-0.36	149.6	1	150.5	-0.36	150.1
2	151.0	-0.36	150.6	2	150.0	-0.36	149.6	2	150.8	-0.36	150.4
3	150.9	-0.36	150.5	3	150.7	-0.36	150.3	3	149.8	-0.36	149.4
		Mean	150.54			Mean	149.87			Mean	150.01
		SD	0.100			SD	0.404			SD	0.513
		%RSD	0.066			%RSD	0.270			%RSD	0.342

Hole 7				Hole 8				Hole 9			
NO.	Result			NO.	Result			NO.	Result		
	temp. °C	Corr.	temp+Corr.		temp. °C	Corr.	temp+Corr.		temp. °C	Corr.	temp+Corr.
1	150.8	-0.36	150.4	1	151.1	-0.36	150.7	1	150.2	-0.36	149.8
2	150.9	-0.36	150.5	2	150.7	-0.36	150.3	2	150.2	-0.36	149.8
3	151.0	-0.36	150.6	3	151.1	-0.36	150.7	3	149.9	-0.36	149.5
		Mean	150.54			Mean	150.61			Mean	149.74
		SD	0.100			SD	0.231			SD	0.173
		%RSD	0.066			%RSD	0.153			%RSD	0.116

Hole 10				Hole 11				Hole 12			
NO.	Result			NO.	Result			NO.	Result		
	temp. °C	Corr.	temp+Corr.		temp. °C	Corr.	temp+Corr.		temp. °C	Corr.	temp+Corr.
1	150.6	-0.36	150.2	1	150.5	-0.36	150.1	1	150.9	-0.36	150.5
2	150.5	-0.36	150.1	2	150.9	-0.36	150.5	2	150.0	-0.36	149.6
3	149.9	-0.36	149.5	3	151.1	-0.36	150.7	3	150.5	-0.36	150.1
		Mean	149.97			Mean	150.47			Mean	150.11
		SD	0.379			SD	0.306			SD	0.451
		%RSD	0.252			%RSD	0.203			%RSD	0.300

Verified By

Approved By

Confidential - Not to be photocopied except by permission of the Laboratory Quality Manager or nominee.

สรุปผลการ Verify

ปรับอุณหภูมิ 154.0 °C แต่ค่าควบคุมมีอุณหภูมิ 150 ± 2 °C ทุกครั้ง

Verified By



Approved By



Confidential - Not to be photocopied except by permission of the Laboratory Quality Manager or nominee.



ARCHEMICA

Certificate of Calibration

Aquion RFIC : Anion System (ID#1054)

**This certificate is to verify that instrument below are calibrated
by**

Archemica Lab Co.,Ltd.

Aquion

S/N 220380025

AS-DV

S/N 2203880170

For

SGS (Thailand) Limited (Rayong Branch).



ARCHEMICA LAB

บริษัท อาร์เคมีกา แล็บ จำกัด

Operator Signa



Date: 15 / Nov / 2023

Applications Chemist



MAINTENANCE AND TEST CERTIFICATE MODEL

Avio220 Max

Customer : <u>SGS(Thailand)Limited</u> <u>Rayong Branch</u> Address : <u>1/209 , 1/211 Moo 1,</u> <u>T. Banchang, A. Banchang</u> <u>Rayong 21130</u> User Name [REDACTED] Phone: [REDACTED] Email: [REDACTED]	Date Tested: <u>January 10, 2024</u> Recommendation Recertification Period <u>6</u> Months Recertification Due: <u>July 10, 2024</u> Date Last Certified: <u>N/A</u> Visit Number: <u>1OF2 W</u> PerkinElmer Phone: <u>02-719-6420 ext 206</u> PerkinElmer Fax: <u>02-318-5597</u>
--	--

CONFIGURATION TESTED

MODEL	SERIAL NUMBER	SOFTWARE
AVIO200 MAX	M79S2304111	Syngristix V5
TESTED EQUIPMENT	CALIBRATION NUMBER	EXPIRATION
IPV Methods		
TEST STANDARD USED	PART NUMBER	EXPIRATION DATE
Multielement Standard	N069-1579	30-Dec-24
Instrument Cal. STD4	N930-0221	30-Nov-24
CUSTOMER SUPPLIED	COMMENTS	CUSTOMER INITIALS
2 % HNO3		
10 % HNO3		



MAINTENANCE AND TEST CERTIFICATE MODEL
Avio220 Max

SERIAL NUMBER <u>M79S2304111</u>	DATE TESTED <u>January 10, 2024</u>
1. MECHANICAL CHECKS	
A. Inspect and clean all fans and filters.	<input type="checkbox"/> OK
B. Inspect and replace as necessary, all torch components including the RF coil.	<input type="checkbox"/> OK
C. Inspect all tubing for sign of clacking or leaking.	<input type="checkbox"/> OK
D. Adjust water and gas pressure regulator settings.	<input type="checkbox"/> OK
E. Inspect and leak check pneumatics drawers.	<input type="checkbox"/> OK
F. Clean the exterior of the instrument.	<input type="checkbox"/> OK
2. OPTICAL CHECKS	
A. Inspect and clean all optical components.	<input type="checkbox"/> OK
B. As required, check and replace all purgebfilters.	<input type="checkbox"/> OK
C. Recheck optical alignment.	<input type="checkbox"/> OK
3. COOLING SYSTEM CHECKS	
A. Perform preventive maintenance on chiller.	<input type="checkbox"/> OK
B. Flush out the chiller every year.	<input type="checkbox"/> OK
4. PERFORMANCE CHECKS	
A. Torch View Alignment.	<input type="checkbox"/> OK
B. Wavelength Calibration.	<input type="checkbox"/> OK



MAINTENANCE AND TEST CERTIFICATE MODEL

Avio220 Max

SERIAL NUMBER <u>M79S2304111</u>		DATE TESTED		<u>January 10, 2024</u>	
PARAMETER		SPECIFICATION		FINAL VALUE	
Spectral Resolution : UV					
As	193.696 nm	≤ 0.009	nm	<u>0.00864</u>	nm
Ni	231.604 nm	≤ 0.011	nm	<u>0.01009</u>	nm
Ni	341.476 nm	≤ 0.015	nm	<u>0.01169</u>	nm
Spectral Resolution : VIS					
Ba	455.403 nm	≤ 0.020	nm	<u>0.01776</u>	nm
Precision					
Zn	206.200 nm	% RSD	≤ 1.0 %	<u>0.28</u>	%
Mg	280.271 nm	% RSD	≤ 1.0 %	<u>0.73</u>	%
Mg	285.213 nm	% RSD	≤ 1.0 %	<u>0.61</u>	%
Ba	455.403 nm	% RSD	≤ 1.0 %	<u>0.54</u>	%
Detection Limits : Axial					
Tl	190.801 nm	3(sd)		<u>1.52</u>	ppb
As	193.696 nm	3(sd)		<u>1.4</u>	ppb
Se	196.026 nm	3(sd)		<u>1.53</u>	ppb
Pb	220.353 nm	3(sd)		<u>1.72</u>	ppb
Detection Limits : Radial					
As	193.696 nm	3(sd)		<u>1.69</u>	ppb
Zn	213.857 nm	3(sd)		<u>0.42</u>	ppb
Mn	257.610 nm	3(sd)		<u>0.1</u>	ppb
La	379.478 nm	3(sd)		<u>0.61</u>	ppb
Ba	455.403 nm	3(sd)		<u>0.13</u>	ppb
Ba	493.408 nm	3(sd)		<u>0.1</u>	ppb
BEC : Axial (IB X 1000)/(IS-IB)					
Mn	257.610 nm	≤ 30 ppb		<u>7.83</u>	ppb
BEC : Radial (IB X 1000)/(IS-IB)					
Mn	257.610 nm	≤ 30 ppb		<u>17.57</u>	ppb



MAINTENANCE AND TEST CERTIFICATE MODEL
Avio220 Max

SERIAL NUMBER M79S2304111

DATE TESTED January 10, 2024

Remarks :

Commissioning follow as commissioning performance sheets.

This is to certify that the above tests have been performed and the configuration tested



meets



does not meet

the PerkinElmer Specifications listed on this certificate.

This certificate does not modify PerkinElmer's standard terms and condition of sale,
including warranty terms.

Service Department PerkinElmer Ltd.

Customer Service Engineer





TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000-29 FAX. 0-2719-9484



Cert.No.: 23CHO565

Page.: 1 of 3

Certificate of Calibration

Equipment :	Spectrophotometer
Manufacturer :	Merck
Model :	Prove 100
Serial No. :	1904113676
ID No. :	S2019025
Condition As-Received:	Used Item
Received Date :	21 September 2023
Calibration Date :	21 September 2023
Reference :	2309-0483OC-2
Submitted by :	SGS (Thailand) Limited 1/209, 1/211 Moo 1, Ban Chang, Ban Chang, Rayong 21130
Calibration Place :	Spectrophotometry Lab
Ambient Temperature :	(23.8 - 20.9) °C (On-Site)
Relative Humidity :	(50.1 - 50.2) % (On-Site)
Calibration Procedure :	In - house method : CP-OCH4 based on ASTM E 275-01

Calibrated by :

Approved by :

26 September 2023

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

A 0058836



Cert. No. : 23CHO565

Page : 2 of 3

Condition of calibration result

1. Reference Standard Material :

<u>Material</u>	<u>Serial No.</u>	<u>Certificate No.</u>	<u>Due date</u>
1. Absorbance Standard set	39130	106269	10 Oct 2024
2. Wavelength Standard set	36730	98330	19 Jan 2024
3. Wavelength Standard set	36730	98331	19 Jan 2024

2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certificate is traceable to the International System of Unit maintained through :
- Starna Scientific Ltd.

4. Spectral BandWidth : 4 nm
Scan Speed : - nm/min

Calibration Results : without adjustment

Wavelength Accuracy

Certified Values of Reference Material (nm)	UUC Reading (nm)	Uncertainty of Measurement (\pm nm)	Coverage Factor <i>k</i>
418.48	418.5	0.15	2.00
513.70	513.1	0.14	2.00
536.90	536.3	0.14	2.00
637.94	637.6	0.14	2.00
879.70	878.8	0.15	2.00



Cert. No. : 23CHO565

Page : 3 of 3

Calibration Results : without adjustment

Photometric Accuracy

Wavelength (nm)	Certified Values of Reference Material (Abs)	UUC Reading (Abs)	Uncertainty of Measurement (\pm Abs)	Coverage Factor <i>k</i>
440.0	Zero	0.000	0.0028	2.00
	0.5645	0.563	0.0028	2.00
	0.6988	0.698	0.0028	2.00
	1.0017	1.001	0.0028	2.00
546.1	Zero	0.000	0.0028	2.00
	0.5281	0.527	0.0028	2.00
	0.6962	0.696	0.0028	2.00
	0.9984	0.998	0.0028	2.00
635.0	Zero	0.000	0.0028	2.00
	0.5699	0.569	0.0028	2.00
	0.7606	0.760	0.0028	2.00
	1.0927	1.092	0.0028	2.00

Remark

- Each individual filter is measured against the empty filter holder (blank) used to zero the spectrophotometer

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k* , providing a level of confidence of approximately 95 %.

-o0o-