JIRANATEE ASSOCIATES CO.,LTD.

[redacted]

Accredited calibration laboratory
ISO/IEC 17025:2017
NSC-TISI-TIS 17025
CALIBRATION 0367

Flow measurement laboratory
Calibration services department.

NSC – TISI – TIS 17025
CALIBRATION 0367

CERTIFICATE OF CALIBRATION

Certificate No. : **COF-044-67**

MEASUREMENT ITEM	: Top Load Orifice
MANUFACTURER	: TISCH
MODEL/TYPE	: TE-5028
SERIAL NUMBER	: 3945
ID NUMBER	: TNP-F-CAL02
CONDITION AS-RECEIVED	: Used item
CUSTOMER	: TNP Environment Co., Ltd. 332/173 Vision Smart Life Village, Bangrak Phatthana, Bang Bua Thong District, Nonthaburi 11110
RECEIVED DATE	: 29 Oct 2024
MEASUREMENT DATE	: 30 Oct 2024
ISSUE DATE	: 30 Oct 2024

Calibration procedure:
The Orifice gas flow device was calibrated against Standard Rotary Displacement Meter (Roots Meter) Model G65/IMC/W2-dp. The WI-CL-004 was used as a calibration guideline.

Traceability:
This certificate provides a traceability of the measurement to recognized the national standards, and to realization of the international system of units (SI) through the NIMT (National Metrology Institute of Thailand) via Certificate number: MW-0063-23.

Uncertainty of Measurement:
The reported uncertainty of measurement is based on the standard uncertainty multiplied by a coverage factor k=2, Which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty has been determined in accordance with the GUM 'Evaluation of measurement data - Guide to the expression of uncertainty in measurement'

ENVIRONMENTAL CONDITIONS:
Ambient condition in the laboratory are as follow:

Temperature	: 23.0 ± 3.0	°C
Relative Humidity	: 55.0 ± 15.0	%RH
Atmospheric Pressure	: 1010 ± 10	hPa

CALIBRATION CONDITION:

Preconditioning	: 24 hours at ambient conditions.
Measurement Condition	: The average values during measurement are 23.9 °C and 55.8 %RH.

NOTED: *The certificate is valid only to the item calibrated on date and place of calibration.*

TABULATION OF RESULTS:
The table on next page give the measured values.

[redacted]

JIRANATEE ASSOCIATES CO.,LTD.

Approved signatory: [redacted]

THIS CERTIFICATE REPORT MAY NOT BE REPRODUCED EXCEPT IN FULL UNLESS PERMISSION FOR REPRODUCTION HAS BEEN OBTAINED IN WRITING FROM THE LABORATORY

JIRANATEE ASSOCIATES CO.,LTD.

MEASUREMENT RESULTS:

The Orifice gas flow device was calibrated by direct comparison method with the Standard Rotary Displacement Meter (Roots Meter). The Humid air was used as a medium in the system. The standard conditions are 25°C (298.15 K) and 760 mmHg for standard temperature and standard pressure respectively.

Table 1: The results of Q Standard calibration data

Plate	Flow rate m^3/min	Pressure [Pa] mmHg	Temperature [Ta] °C	Temperature [Tm] °C	Δp_meter mmHg	Δp_Orifice inH_2O	Y	Standard Flow [Q_s] m^3/min
1	0.703	758.163	23.78	22.67	49.921	1.158	1.077	0.660
2	0.999	758.204	23.26	22.30	35.795	2.480	1.577	0.959
3	1.117	758.225	23.29	22.38	30.579	3.143	1.776	1.079
4	1.164	758.281	23.31	22.57	28.519	3.425	1.854	1.127
5	1.414	758.199	23.33	22.86	18.318	5.237	2.292	1.387

Slope (m): **1.66978**

Intercept (b): **-0.02500**

Correlation coefficient (r): **0.99989**

Uncertainty (k=2): **0.015** **m^3/min**

Table 2: The results of Q actual calibration data

Plate	Flow rate m^3/min	Pressure [Pa] mmHg	Temperature [Ta] °C	Temperature [Tm] °C	Δp_meter mmHg	Δp_Orifice inH_2O	Y	Standard Flow [Q_a] m^3/min
1	0.703	758.163	23.78	22.67	49.921	1.158	0.673	0.659
2	0.999	758.204	23.26	22.30	35.795	2.480	0.985	0.955
3	1.117	758.225	23.29	22.38	30.579	3.143	1.109	1.075
4	1.164	758.281	23.31	22.57	28.519	3.425	1.157	1.123
5	1.414	758.199	23.33	22.86	18.318	5.237	1.431	1.382

Slope (m): **1.04588**

Intercept (b): **-0.01565**

Correlation coefficient (r): **0.99989**

Uncertainty (k = 2): **0.015** **m^3/min**

*****End of Certificate of Calibration*****

JIRANATEE ASSOCIATES CO.,LTD.

Jiranatee Associates Co., Ltd.

ENVIR SERVICE CO., LTD.
42 Ramintra 14 Yeak 9, Tha Raeng, Bang Khen, Bangkok 10230
Tel. 02-9435814-5 Fax. 02-9438201 www.envirservice.co.th

CALIBRATION TEST REPORT FOR Partisol® Model 2000 Air Sampler

Calibrated Date: 10 October 2024
Calibrated Due on: 09 October 2025

Report No: PM-202410011

Instruments Information

Description : Thermo Scientific Partisol FRM 2000 Air Sampler for PM-2.5
Model : 2000
Sample flow control and reporting : 5 - 18 L/min
Serial No. : 200FB205150107


Instrument used for calibration [STD]

Description : Flow Meter BIOS DryCal DC-Lite
Model : DCL-M REV. 1.08
Range : 200 ml/min - 20 L/min
Serial No. : 1519

Environment : Temperature 25.5 ˚C Humidity: 51 %RH

Calibration Report

Filter	Set Flow Instrument (L/Min)	Current Flow Instrument reading (L/Min)	Actual Flow Reference standard (L/Min)	Flow Offset	Flow Span
47 mm.	16.7	16.6	16.7	0.0078	1.0000
	17.5	17.2	17.4	0.0078	0.9618
	15.8	15.8	15.7	0.0078	0.9534
	18.3	18.3	18.3	0.0078	0.9540
	15.0	15.0	15.1	0.0078	0.9633

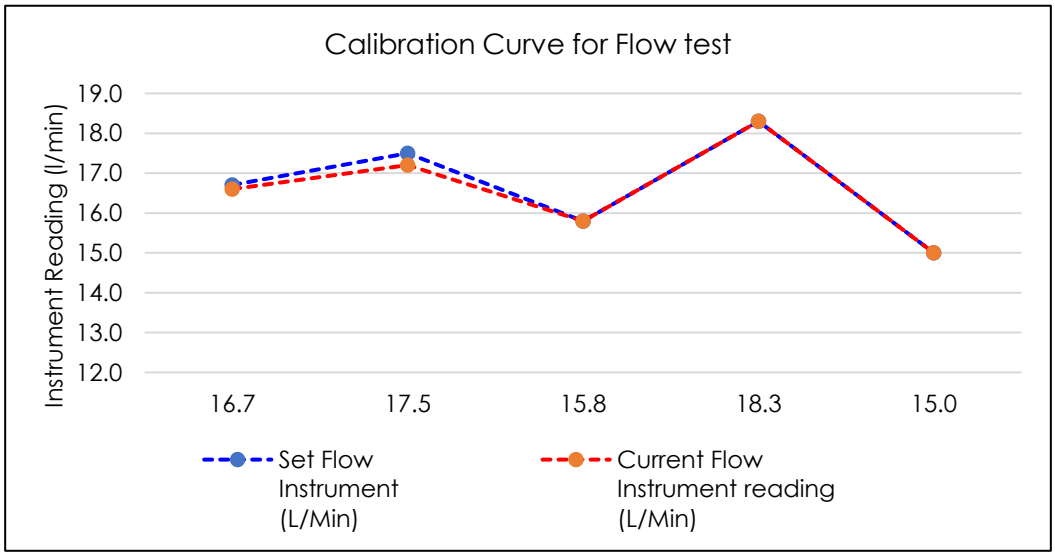

Calibrate By : [redacted]

ENVIR SERVICE CO., LTD.
42 Ramintra 14 Yeak 9, Tha Raeng, Bang Khen, Bangkok 10230
Tel. 02-9435814-5 Fax. 02-9438201 www.envirservice.co.th

Analyzer Performance Test

Calibrated Date: 08 November 2024

Instruments Information

Analyzer Type : CO Analyzer
Model : 48C
Manufacturer : Thermo Environmental
Serial Number : 48C-67530-357

Calibrator Unit
Dilutor Model : Dasibi Model 5008
Serial Number : 705
ZERO AIR Genearator : API MODEL 701
Serial Number : 1924


Standard Gas Concentration

Nitric Oxide (NO)	55.47	PPM
Sulphur Dioxide (SO2)	55.11	PPM
Carbon Monoxide (CO)	4,535	PPM
Cylinder number	EB0129027	
Expire Date:	29 Oct. 2027	

Environment : Temperature 25.5 °C Humidity: 51 %RH

Calibration Report

	Zero			Span		
	Reference (PPM)	Reading (PPM)	Drift (PPM)	Reference (PPM)	Reading (PPM)	Drift%
Before	0.0	0.2	0.2	45.0	44.2	-1.8
After	0.0	0.0	0.0	45.0	45.0	0.0

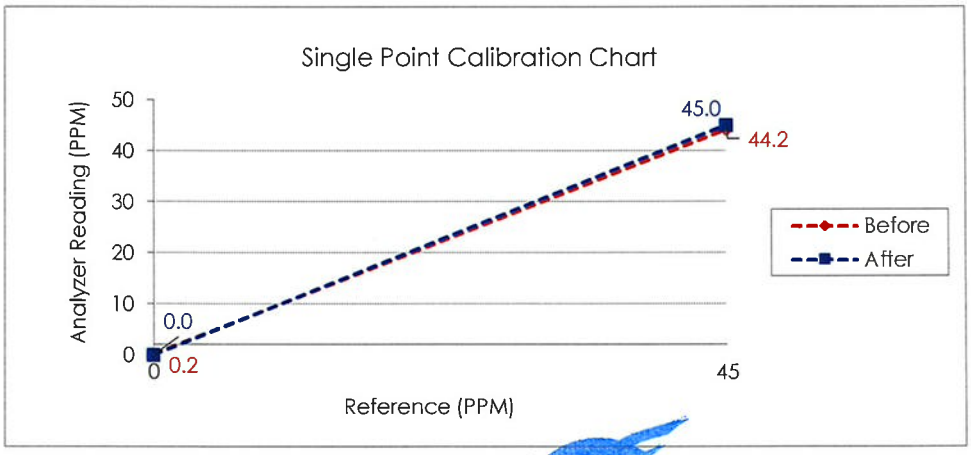

Calibrate By [redacted]

ENVIR SERVICE CO., LTD

ENVIR SERVICE CO., LTD.
42 Ramintra 14 Yeak 9, Tha Raeng, Bang Khen, Bangkok 10230
Tel. 02-9435814-5 Fax. 02-9438201 www.envirservice.co.th

Analyzer Performance Test

Calibrated Date: 25 October 2024

Instruments Information

Analyzer Type : CO Analyzer
Model : 48C
Manufacturer : Thermo Environmental
Serial Number : 48CHL-67713-358

Calibrator Unit
Dilutor Model : Dasibi Model 5008
Serial Number : 705
ZERO AIR Genearator : API MODEL 701
Serial Number : 1924


Standard Gas Concentration

Nitric Oxide (NO)	55.47	PPM
Sulphur Dioxide (SO2)	55.11	PPM
Carbon Monoxide (CO)	4,535	PPM
Cylinder number	EB0129027	
Expire Date:	29 Oct. 2027	

Environment : Temperature 25.5 ˚C Humidity: 51 %RH

Calibration Report

	Zero			***Span***		
	Reference (PPM)	Reading (PPM)	Drift (PPM)	Reference (PPM)	Reading (PPM)	Drift%
Before	0.0	0.2	0.2	45.0	44.2	-1.8
After	0.0	0.0	0.0	45.0	45.0	0.0

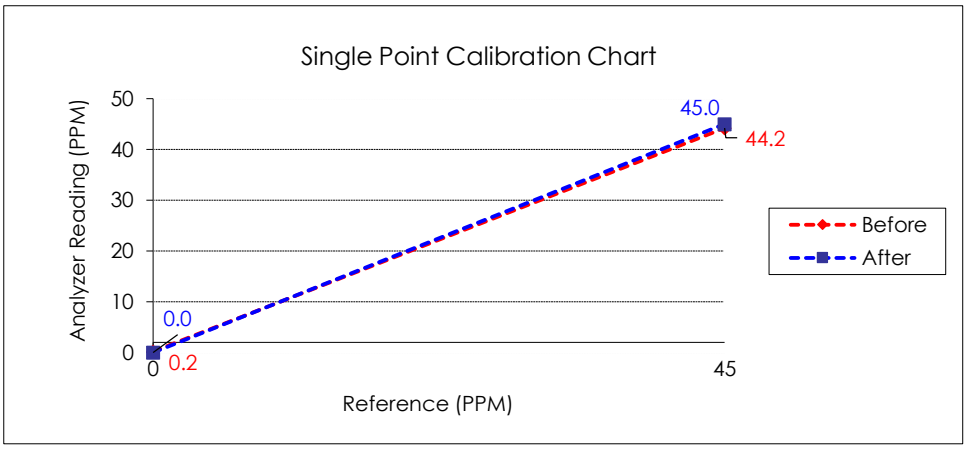

Calibrate By : [redacted]

ENVIR SERVICE CO., LTD.
42 Ramintra 14 Yeak 9, Tha Raeng, Bang Khen, Bangkok 10230
Tel. 02-9435814-5 Fax. 02-9438201 www.envirservice.co.th

Analyzer Performance Test

Calibrated Date: 14 August 2024

Instruments Information

Analyzer Type : NO-NO2-NOx Analyzer
Manufacturer : Thermo Environmental
Model : 42C
Serial Number : 42C-59194-321

Calibrator Unit
Dilutor Model : Dasibi Model 5008
Serial Number : 705
ZERO AIR Genearator : API MODEL 701
Serial Number : 1924

Standard Gas Concentration

Nitric Oxide (NO)	55.47	PPM
Sulphur Dioxide (SO2)	55.11	PPM
Carbon Monoxide (CO)	4,535	PPM
Cylinder number	EB0129027	
Expire Date:	29 Oct. 2027	


Environment : Temperature 25.5 ˚C Humidity: 51 %RH

Calibration Report (Before Adjust)

Status	Zero			Span		
	Reference (PPB)	Reading (PPB)	Drift (PPB)	Reference (PPB)	Reading (PPB)	Drift%
NO	0.0	0.1	0.1	400.0	393.3	-1.7
NOx	0.0	0.0	0.0	400.0	393.6	-1.6

Calibration Report (After Adjust)

Status	Zero			Span		
	Reference (PPB)	Reading (PPB)	Drift (PPB)	Reference (PPB)	Reading (PPB)	Drift%
NO	0.0	0.1	0.1	400.0	400.0	0.0
NOx	0.0	0.0	0.0	400.0	400.0	0.0

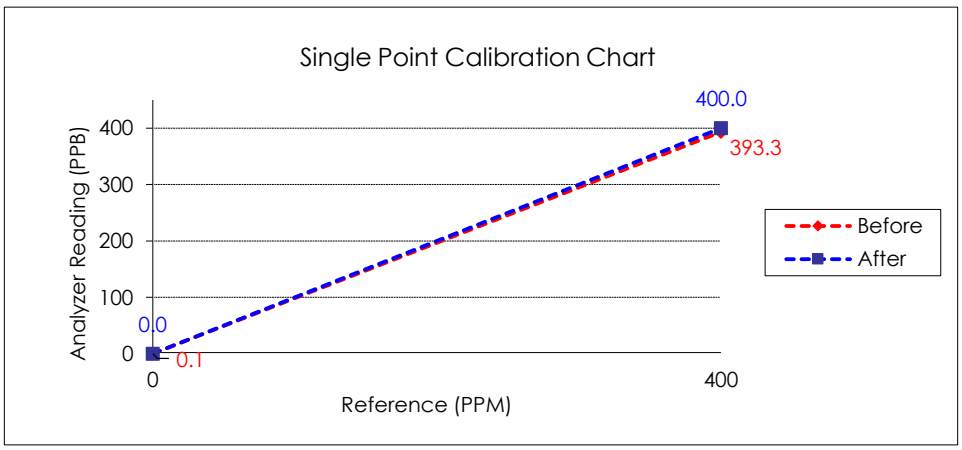

Calibrate By : [redacted]

ENVIR SERVICE CO., LTD.
42 Ramintra 14 Yeak 9, Tha Raeng, Bang Khen, Bangkok 10230
Tel. 02-9435814-5 Fax. 02-9438201 www.envirservice.co.th

Analyzer Performance Test

Calibrated Date: 08 November 2024

Instruments Information

Analyzer Type : NO-NO2-NOx Analyzer
Manufacturer : Thermo Environmental
Model : 42C
Serial Number : 42C-70987-367

Calibrator Unit
Dilutor Model : Dasibi Model 5008
Serial Number : 705
ZERO AIR Genearator : API MODEL 701
Serial Number : 1924

Standard Gas Concentration

Nitric Oxide (NO)	55.47	PPM
Sulphur Dioxide (SO2)	55.11	PPM
Carbon Monoxide (CO)	4,535	PPM
Cylinder number	EB0129027	
Expire Date:	29 Oct. 2027	


Environment : Temperature 25.5 °C Humidity: 51 %RH

Calibration Report (Before Adjust)

Status	Zero			Span		
	Reference (PPB)	Reading (PPB)	Drift (PPB)	Reference (PPB)	Reading (PPB)	Drift%
NO	0.0	0.1	0.1	400.0	393.1	-1.7
NOx	0.0	0.0	0.0	400.0	393.3	-1.7

Calibration Report (After Adjust)

Status	Zero			Span		
	Reference (PPB)	Reading (PPB)	Drift (PPB)	Reference (PPB)	Reading (PPB)	Drift%
NO	0.0	0.1	0.1	400.0	400.0	0.0
NOx	0.0	0.0	0.0	400.0	400.0	0.0

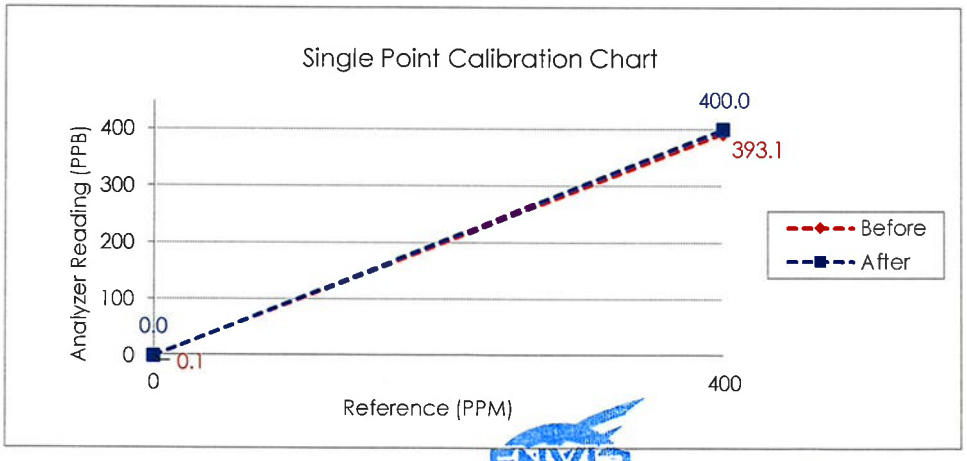

Calibrate By : [redacted]

ENVIR SERVICE CO., LTD.
42 Ramintra 14 Yeak 9, Tha Raeng, Bang Khen, Bangkok 10230
Tel. 02-9435814-5 Fax. 02-9438201 www.envirservice.co.th

Analyzer Performance Test

Calibrated Date: 07 November 2024

Instruments Information

Analyzer Type : SO2 Analyzer
Model : 43C
Manufacturer : Thermo Environmental
Serial Number : 43C-0427408948

Calibrator Unit
Dilutor Model : Dasibi Model 5008
Serial Number : 705
ZERO AIR Genearator : API MODEL 701
Serial Number : 1924


Standard Gas Concentration

Nitric Oxide (NO)	55.47	PPM
Sulphur Dioxide (SO2)	55.11	PPM
Carbon Monoxide (CO)	4,535	PPM
Cylinder number	EB0129027	
Expire Date:	29 Oct. 2027	

Environment : Temperature 25.5 °C Humidity: 51 %RH

Calibration Report

Status	Zero			Span		
	Reference (PPB)	Reading (PPB)	Drift (PPB)	Reference (PPB)	Reading (PPB)	Drift%
Before	0.0	0.1	0.1	400.0	393.2	-1.7
After	0.0	0.0	0.0	400.0	400.0	0.0

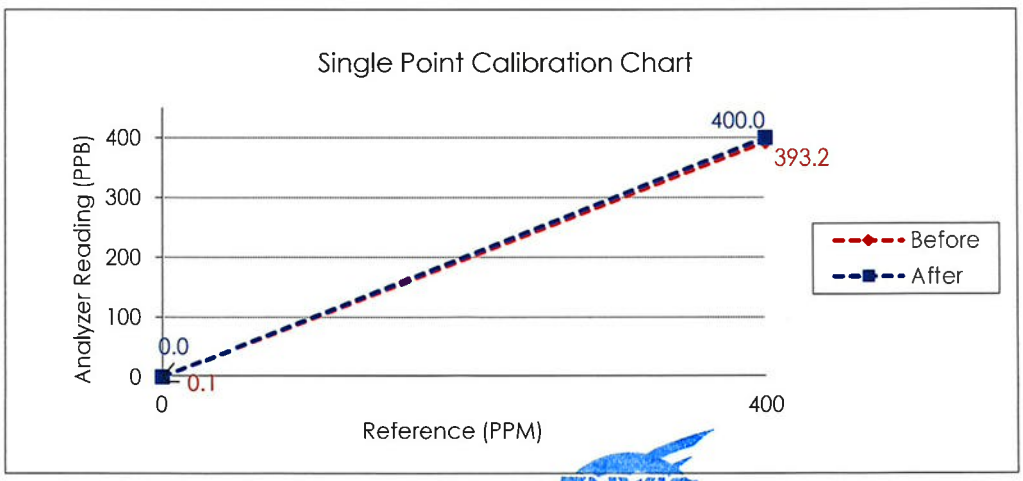

Calibrate By : [redacted]

ENVIR SERVICE CO., LTD.
42 Ramintra 14 Yeak 9, Tha Raeng, Bang Khen, Bangkok 10230
Tel. 02-9435814-5 Fax. 02-9438201 www.envirservice.co.th

Analyzer Performance Test

Calibrated Date: 14 August 2024

Instruments Information

Analyzer Type : SO2 Analyzer
Manufacturer : Thermo Environmental
Model : 43C
Serial Number : 43C-71079-367

Calibrator Unit
Dilutor Model : Dasibi Model 5008
Serial Number : 705
ZERO AIR Genearator : API MODEL 701
Serial Number : 1924


Standard Gas Concentration

Nitric Oxide (NO)	55.47	PPM
Sulphur Dioxide (SO2)	55.11	PPM
Carbon Monoxide (CO)	4,535	PPM
Cylinder number	EB0129027	
Expire Date:	29 Oct. 2027	

Environment : Temperature 25.5 ˚C Humidity: 51 %RH

Calibration Report

Status	Zero			Span		
	Reference (PPB)	Reading (PPB)	Drift (PPB)	Reference (PPB)	Reading (PPB)	Drift%
Before	0.0	0.1	0.1	400.0	393.1	-1.7
After	0.0	0.0	0.0	400.0	400.0	0.0

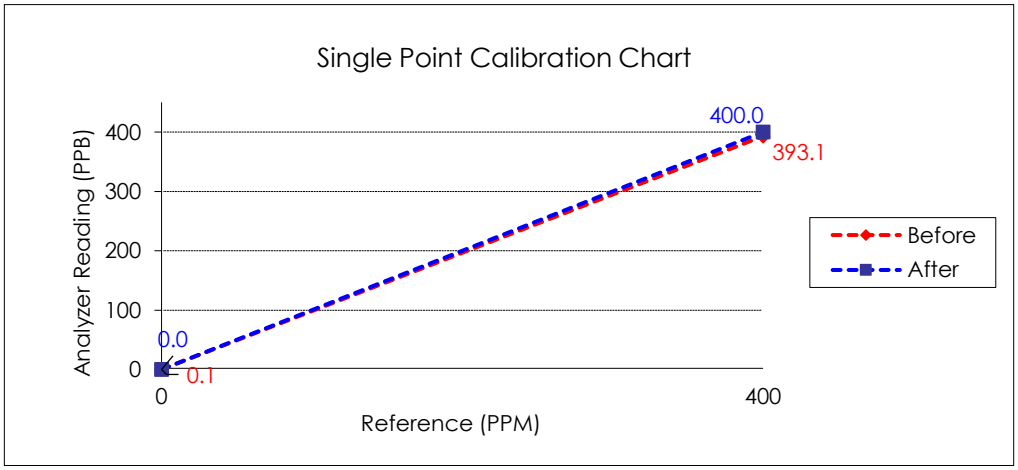

Calibrate By : [redacted]

ENVIR SERVICE CO., LTD.
42 Ramintra 14 Yeak 9, Tha Raeng, Bang Khen, Bangkok 10230
Tel. 02-9435814-5 Fax. 02-9438201 www.envirservice.co.th

Analyzer Performance Test

Calibrated Date: 2023-Nov-1

Instruments Information

Analyzer Type : CH4-NMHC-THC Analyzer
Manufacturer : HORIBA
Model : APHA-360CE
Serial Number : 423740300209

Calibrator Unit
Dilutor Model : Dasibi Model 5008
Serial Number : 705
ZERO AIR Genearator : API MODEL 701
Serial Number : 1924

Standard Gas Concentration
Methane (CH4) 181.0 PPM
Propane 180.7 PPM
Cylinder number EB0123130
Expire Date: 3 Oct. 2027


Environment : Temperature 25.5 ˚C Humidity: 51 %RH

Calibration Report (Before adjust)

Status	Zero			Span		
	Reference (PPM)	Reading (PPM)	Drift (PPM)	Reference (PPM)	Reading (PPM)	Drift%
Methane	0.0	0.1	0.1	50.0	49.1	-1.8
NMHC	0.0	0.1	0.1	50.0	48.9	-2.2

Calibration Report (After adjust)

Status	Zero			Span		
	Reference (PPM)	Reading (PPM)	Drift (PPM)	Reference (PPM)	Reading (PPM)	Drift%
Methane	0.0	0.0	0.0	50.0	50.0	0.0
NMHC	0.0	0.0	0.0	50.0	50.0	0.0

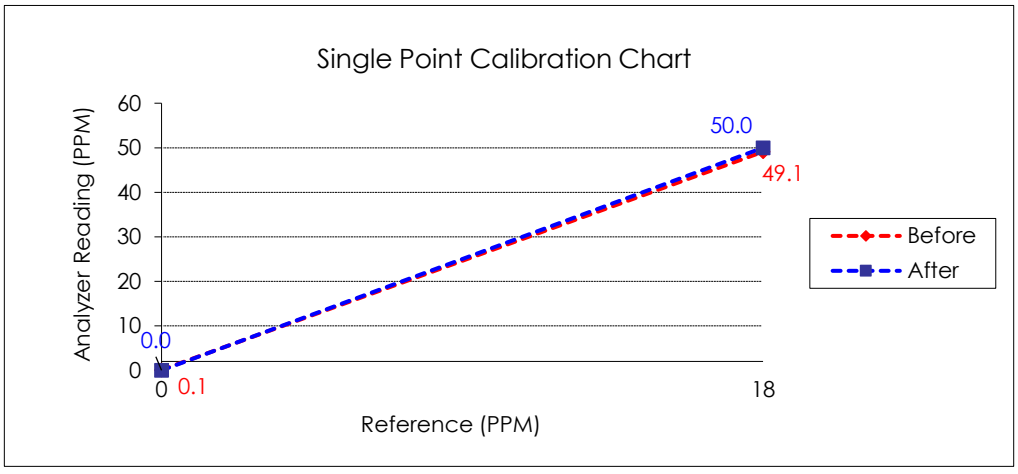

Calibrate By : [redacted]

THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-67/0575 **MTC No.** EEL. BP. 15/0867

CALIBRATION CERTIFICATE

Submitted by : TNP ENVIRONMENT CO.,LTD.

Address : 332/173 Moo 3 Bang Rak Phatthana, Bang Bua Tong, Nonthaburi 11110.

Calibrated at : Electrical and Electronic Standards Laboratory, Industrial Metrology and Testing Service Centre.
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Rd., Muang, Samutprakan 10280.

Instrument Calibrated :

Description : Sound Calibrator

Manufacturer : KEPLER

Model : KSM-42C

Serial No. : 160100568

Ambient Environment

Temperature : (23 ± 3) °C

Relative Humidity : (50 ± 15) %

Ambient Pressure : (101.325 ± 1.500) kPa

Standards used :

1. Digital Function Synthesizer NF Electronic DF-193A S/N 122037.
2. Measuring Amplifier Bruel&Kjaer 2636 S/N 1537484.
3. Programmable Attenuator Tamagawa TPA-303A S/N OF 2214.
4. Digital Multimeter Agilent 34401A S/N MY44005560.
5. Pressure Transmitter Vaisala PTB202AD S/N T0650001.
6. Audio Analyzer Panasonic VP-7722A S/N 041477D122.
7. Condenser Microphone B&K 4180 S/N 2633526.

Calibration Procedure: CP-102-04 based on IEC 60942-2003. The sound pressure level of instrument was measured by standard microphone using an insert voltage technique.

This instrument has been calibrated against standards maintained at Electrical and Electronic Standards Laboratory (EEL), which are traceable to the International System of Units through the National Institute of Metrology (Thailand).

The information on actual reading is attached herewith and the uncertainty limits quoted refer to the measured values only.

Date of Receipt : 6 Aug. 2024

Date of Calibration : 26 Aug. 2024

The results relate only to the items tested/calibrated or value assigned.
Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9009

Office/Laboratory
668 Mu 2 Tambon Bangpoomai, Amphoe Muang Samutprakan,
Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtc@tistr.or.th Website : www.tistr.or.th

Office
196 Phahonyothin Road, Ladyao, Chatuchak,
Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827

THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-67/0575 **MTC No.** EEL. BP. 15/0867

The reported expanded uncertainty is based upon a standard uncertainty multiplied by a coverage factor k = 2, providing a level of confidence of approximately 95%.

Nominal Output of Unit Under Test = 94 dB re 20μPa at 1000 Hz

Acoustic Output in dB re 20μPa , Corrected to Reference Conditions : 101.325 kPa , 23.0°C and 50 %RH

1. Sound Pressure Level

Standard Microphone Type	Measured Sound Pressure Level (dB)	Deviated value (dB)	Uncertainty (dB)	Tolerance limit IEC60942:2003 Class 2
1/2 inch Bruel&Kjaer 4180	94.30	0.30	± 0.10	±0.75 dB

2. Frequency

Standard Microphone Type	Measured Frequency (Hz)	Deviated value (Hz)	Uncertainty (Hz)	Tolerance limit IEC60942:2003 Class 2
1/2 inch Bruel&Kjaer 4180	969.9	-30.1	± 1.5	±2.0%

3. Total distortion

Standard Microphone Type	Measured Total distortion (%)	Uncertainty (%)	Tolerance limit IEC60942:2003 Class 2
1/2 inch Bruel&Kjaer 4180	1.70	± 0.50	±4.0%

Note : 1. No adjustment.

2. The calibrator pressure correction was not included.

3. The microphone volume correction was not included.

Date of Calibration : 26 Aug. 2024

[redacted]

The results relate only to the items tested/calibrated or value assigned.
Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9009

Office/Laboratory
668 Mu 2 Tambon Bangpoomai, Amphoe Muang Samutprakan,
Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtc@tistr.or.th Website : www.tistr.or.th

Office
196 Phahonyothin Road, Ladyao, Chatuchak,
Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827

THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-67/0575 **MTC No.** EEL. BP. 15/0867

Nominal Output of Unit Under Test = 114 dB re 20µPa at 1000 Hz

Acoustic Output in dB re 20µPa , Corrected to Reference Conditions : 101.325 kPa , 23.0 °C and 50 %RH

1. Sound Pressure Level

Standard Microphone Type	Measured Sound Pressure Level (dB)	Deviated value (dB)	Uncertainty (dB)	Tolerance limit IEC60942:2003 Class 2
1/2 inch Bruel&Kjaer 4180	114.33	0.33	± 0.10	±0.75 dB

2. Frequency

Standard Microphone Type	Measured Frequency (Hz)	Deviated value (Hz)	Uncertainty (Hz)	Tolerance limit IEC60942:2003 Class 2
1/2 inch Bruel&Kjaer 4180	965.6	-34.4	± 1.5	±2.0%

3. Total Distortion

Standard Microphone Type	Measured Total Distortion (%)	Uncertainty (%)	Tolerance limit IEC60942:2003 Class 2
1/2 inch Bruel&Kjaer 4180	2.15	± 0.50	±4.0%

Note : 1. No adjustment.

2. The calibrator pressure correction was not included.

3. The microphone volume correction was not included.

Calibrated by : [redacted]

Approved by [redacted]

Director

Electrical and Electronic Standards Laboratory

Industrial Metrology and Testing Service Centre

Date of Calibration : 26 Aug. 2024

Date of Issue : 27 Aug. 2024

Ref : 2011167080602911001

End of Certificate

The results relate only to the items tested/calibrated or value assigned.
Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9009

Office/Laboratory
668 Mu 2 Tambon Bangpoomai, Amphoe Muang Samutprakan,
Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtc@tistr.or.th Website : www.tistr.or.th

Office
196 Phahonyothin Road, Ladyao, Chatuchak,
Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827

SMART TECH CALIBRATION & SERVICES CO., LTD.
14/506 MOO 3, RANGSIT-NAKHON NAYOK ROAD, LAM PHAK KUT,
THANYABURI, PATHUM THANI 12110, THAILAND
Tel. +662-114-3148 Email : stcal.md@gmail.com Website : stc-cal.com

ANAB ACCREDITED ISO/IEC 17025 CALIBRATION LABORATORY AC-3093

Certificate of Calibration

Certificate No. STCR-2407092-1
Work Order No. STCR-2407092

Customer Name	:	TNP Environment Co., Ltd. 332/173 Vision Smart Life Village, Bang Rak Pattana Subdistrict, Bang Bua Thong District, Nonthaburi Province 11110
Equipment Name	:	Sound Level Meter
Manufacturer	:	SCARLET
Model	:	ST-25D
Serial Number	:	10340945
Control Number	:	TNP-F-S25
Received Date	:	Jul 4, 2024
Calibration Date	:	Jul 5, 2024
Recommended Due Date	:	Jul 5, 2025
Calibration Method	:	Calibration Procedure No. CPE-04-01
Environmental Conditions		
Ambient Temperature	:	(25 ± 2) °C
Ambient Relative Humidity	:	(50 ± 15) %RH
Calibration Place	:	Permanent Calibration Laboratory
Condition as received	:	Normal
Calibration Result	:	See data attached

1. The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor k = 2, providing a level of confidence of approximately 95%.
2. The Unit Under Calibration (UUC) has been calibrated by using the working standard which is traceable to SI-Units. The calibration procedure documented is intended to implement the requirements of ISO/IEC 17025 : 2017
3. The working standard is indicated in page 2 of this certificate.
4. This report applies to the item calibrated and shall not be reproduced except in full, without written approval by Calibration Laboratory, Smart Tech Calibration & Services Co., Ltd.
5. This results of this report only to the items calibrated.

Date of Issue
Calibrated by [redacted]

Approved by : [redacted]
Laboratory Manager

@smarttechcal

Calibration Report

Smart Tech Calibration & Services Co., Ltd.

Certificate No.: STCR-2407092-1

Standards Equipment Used

Equipment Name	Serial No.	Certificate No.	Due Date	Traceability to
Sound Calibrator	N975185	5523631030478623	Nov 9, 2024	MP-TH

Traceability

This calibration is traceable to the International System of Unit via :

- MP-TH : Micro Precision Calibration Laboratory (Thailand) Co., Ltd.

STC
TM

Calibration Report

Smart Tech Calibration & Services Co., Ltd.

Certificate No.: STCR-2407092-1

UUC Range : (30 to 130) dB Resolution : 0.1 dB

Results of Calibration: [ ] Without adjustment [✓] With adjustment

Appearance and Function of Use Inspection : GOOD

Sound Level Calibration @ Frequency 1 kHz Select : A

Response times	STD. Value	UUC. Reading		Correction	(±) Uncertainty
		Before Adjustment	After Adjustment		
FAST	94.09 dB	93.2 dB	94.1 dB	-0.01 dB	0.40 dB
	114.07 dB	113.1 dB	114.0 dB	0.07 dB	0.40 dB
SLOW	94.09 dB	93.2 dB	94.1 dB	-0.01 dB	0.40 dB
	114.07 dB	113.1 dB	113.9 dB	0.17 dB	0.40 dB

Sound Level Calibration @ Frequency 1 kHz Select : C

Response times	STD. Value	UUC. Reading		Correction	(±) Uncertainty
		Before Adjustment	After Adjustment		
FAST	94.09 dB	93.2 dB	94.1 dB	-0.01 dB	0.40 dB
	114.07 dB	113.1 dB	114.0 dB	0.07 dB	0.40 dB
SLOW	94.09 dB	93.2 dB	94.1 dB	-0.01 dB	0.40 dB
	114.07 dB	113.2 dB	114.0 dB	0.07 dB	0.40 dB

STD = Standard

UUC = Unit Under Calibration

- End of Certificate -

STC TM

SMART TECH CALIBRATION & SERVICES CO., LTD.
14/506 MOO 3, RANGSIT-NAKHON NAYOK ROAD, LAM PHAK KUT,
THANYABURI, PATHUM THANI 12110, THAILAND
Tel. +662-114-3148 Email : stcal.md@gmail.com Website : stc-cal.com

ANAB ANSI National Accreditation Board ACCREDITED ISO/IEC 17025 CALIBRATION LABORATORY AC-3093

Certificate of Calibration

Certificate No. STCR-2407075-1
Work Order No. STCR-2407075

Customer Name	:	TNP Environment Co., Ltd. 332/173 Vision Smart Life Village, Bang Rak Pattana Subdistrict, Bang Bua Thong District, Nonthaburi Province 11110
Equipment Name	:	Sound Level Meter
Manufacturer	:	Scarlet Tech
Model	:	ST-25D
Serial Number	:	10340943
Control Number	:	TNP-F-S26
Received Date	:	Jul 4, 2024
Calibration Date	:	Jul 5, 2024
Recommended Due Date	:	Jul 5, 2025
Calibration Method	:	Calibration Procedure No. CPE-04-01

Environmental Conditions

Ambient Temperature	:	(25 ± 2) °C
Ambient Relative Humidity	:	(50 ± 15) %RH
Calibration Place	:	Permanent Calibration Laboratory
Condition as received	:	Normal
Calibration Result	:	See data attached

1. The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor k = 2, providing a level of confidence of approximately 95%.
2. The Unit Under Calibration (UUC) has been calibrated by using the working standard which is traceable to SI-Units. The calibration procedure documented is intended to implement the requirements of ISO/IEC 17025 : 2017
3. The working standard is indicated in page 2 of this certificate.
4. This report applies to the item calibrated and shall not be reproduced except in full, without written approval by Calibration Laboratory, Smart Tech Calibration & Services Co., Ltd.
5. This results of this report only to the items calibrated.

Date of Issue
Calibrated by [redacted]
Approved by [redacted]

@smarttechcal

Calibration Report

Smart Tech Calibration & Services Co., Ltd.

Certificate No.: STCR-2407075-1

Standards Equipment Used

Equipment Name	Serial No.	Certificate No.	Due Date	Traceability to
Sound Calibrator	N975185	5523631030478623	Nov 9, 2024	MP-TH

Traceability

This calibration is traceable to the International System of Unit via :

- MP-TH : Micro Precision Calibration Laboratory (Thailand) Co., Ltd.

STC
TM

Calibration Report

Smart Tech Calibration & Services Co., Ltd.

Certificate No.: STCR-2407075-1

UUC Range : (38 to 130) dB Resolution : 0.1 dB

Results of Calibration: [ ] Without adjustment [✓] With adjustment

Appearance and Function of Use Inspection : GOOD

Sound Level Calibration @ Frequency 1 kHz Select : A

Response times	STD. Value	UUC. Reading		Correction	(±) Uncertainty
		Before Adjustment	After Adjustment		
FAST	94.09 dB	93.0 dB	94.0 dB	0.09 dB	0.40 dB
	114.07 dB	112.8 dB	113.9 dB	0.17 dB	0.40 dB
SLOW	94.09 dB	93.0 dB	94.0 dB	0.09 dB	0.40 dB
	114.07 dB	112.8 dB	114.0 dB	0.07 dB	0.40 dB

Sound Level Calibration @ Frequency 1 kHz Select : C

Response times	STD. Value	UUC. Reading		Correction	(±) Uncertainty
		Before Adjustment	After Adjustment		
FAST	94.09 dB	93.0 dB	94.0 dB	0.09 dB	0.40 dB
	114.07 dB	112.8 dB	113.9 dB	0.17 dB	0.40 dB
SLOW	94.09 dB	93.0 dB	94.1 dB	-0.01 dB	0.40 dB
	114.07 dB	112.8 dB	114.0 dB	0.07 dB	0.40 dB

STD = Standard

UUC = Unit Under Calibration

- End of Certificate -

STC
TM

CALIBRATION LABORATORY CO., LTD.
2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com

CLC
Accredited
ISO/IEC 17025

ANAB
ANSI National Accreditation Board
ACCREDITED
ISO/IEC 17025
CALIBRATION AND DIMENSIONAL MEASUREMENT
ACDM-2814

CERTIFICATE OF CALIBRATION

FOR

NOMENCLATURE	:	VIBRATION METER
MANUFACTURER	:	INSTANTEL
MODEL / TYPE	:	721A2601/721A3301
SERIAL NO.	:	UM14102/UM14102
CLID. NO.	:	252100393
JOB CONTROL NO.	:	241101116709
CALIBRATION SERVICE	:	☑ IN-LABORATORY ☐ ON-SITE

CUSTOMER : TNP ENVIRONMENT CO., LTD.
332/173 MOO 3 TAMBON BANG RAK PHATTANA,
AMPHOE BANG BUA THONG, NONTHABURI 11110

DATE OF RECEIVED : 01 November 2024 DATE OF ISSUED : 06 November 2024

The report of calibration shall not be reproduced except in full without approval of the Calibration Laboratory Co., Ltd.

Calibrated By :

[redacted]

Approved By :

06 November 2024

This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to the International System of Units (SI)

Certificate No. Q24116709

@clccalibration

CALIBRATION LABORATORY CO., LTD.
2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com

CLC
Accredited
ISO/IEC 17025

ANAB
ANSI National Accreditation Board
ACCREDITED
ISO/IEC 17025
CALIBRATION AND DIMENSIONAL MEASUREMENT
ACDM-2814

REPORT OF CALIBRATION

FOR

NOMENCLATURE	:	**VIBRATION METER**
MANUFACTURER	:	**INSTANTEL**
MODEL / TYPE	:	**721A2601/721A3301**
SERIAL NO.	:	**UM14102/UM14102**
DATE OF CALIBRATION	:	**04 November 2024**

ENVIRONMENT CONDITIONS :

Temperature : (23 ± 2) °C **Relative Humidity :** (55 ± 15) %RH

PROCEDURE USED :

This instrument was calibrated under procedure No. **CLC-CPEE-08** based on **ISO 16063-21** as calibration guideline.
The calibration was performed by using Digital Multimeter, Programmable Timer/Counter, Vibration Calibrator which maintained by the Calibration Laboratory Co., Ltd.

REFERENCE STANDARD USED :

1. Vibration Calibrator, The Modal Shop Model 9110D S/N. 11424.
2. Digital Multimeter, Hewlett Packard Model 34401A S/N. 3146A75935.
3. Programmable Timer/Counter, Philips Model PM6680B S/N. SM607101.

TRACEABILITY :

1. The measurements are traceable to International System of Units (SI), through National Institute of Metrology (Thailand) Certificate No. AV-0030-24, Due Date 19 July 2025.
2. The measurements are traceable to International System of Units (SI), through National Institute of Metrology (Thailand) Certificate No. EE-0130-23, Due Date 29 November 2024.
3. The measurements are traceable to International System of Units (SI), through Aeronautical Radio of Thailand Ltd. Certificate No. 07-0050/24 , Due Date 13 May 2025 .

UNCERTAINTY :

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor $k = 2{,}00$ which for a normal distribution corresponds to a coverage probability of approximately 95 %.
It has been evaluated according to the "Evaluation of the Uncertainty of Measurement in Calibration (EA-4/02 M:2022)"

@clccalibration

CONDITION OF CALIBRATION ITEM : RECEIVED IN GOOD OPERATIONAL CONDITION

MEASUREMENT RESULTS : (X) without adjustment ( ) adjustment

CALIBRATION DATA

1. VELOCITY RESULT

Test point		Mode	STD Reading	DUC Reading	Correction	Uncertainty
(mm/s)	(frequency)		(mm/s)	(mm/s)	(mm/s)	± (% of rdg.)
10	80 Hz	peak	10.000	10.097	-0.097	1.5
20	80 Hz		20.000	20.188	-0.188	1.5
30	80 Hz		30.000	30.256	-0.256	1.5
40	80 Hz		40.000	40.365	-0.365	1.5
50	80 Hz		50.000	50.421	-0.421	1.5

Note. The Scope of Accredited ANAB Certificate No. ACDM-2814 Version 012 Page 2 of 67

CALIBRATION LABORATORY CO., LTD.
2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com

CLC
Accredited
ISO/IEC 17025

ANAB
ANSI National Accreditation Board
ACCREDITED
ISO/IEC 17025
CALIBRATION AND DIMENSIONAL MEASUREMENT
ACDM-2814

CALIBRATION DATA

*2. FREQUENCY RESULT

STD Applied (Hz)	DUC Reading (Hz)	Correction (Hz)	Uncertainty ± (Hz)
50	50	0	0.6
80	79	+1	0.6
100	100	0	0.6

Note. * means Calibrations marked " Not ANAB Accredited " in this Certificate have been included for completeness.

This report is valid for the above stated instrument/s only.

End of Certificate

@clccalibration

CALIBRATION LABORATORY CO., LTD.
2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com

CLC Accredited ISO/IEC 17025

ANAB ANSI National Accreditation Board ACCREDITED ISO/IEC 17025 CALIBRATION AND DIMENSIONAL MEASUREMENT ACDM-2814

CERTIFICATE OF CALIBRATION

FOR

NOMENCLATURE	:	VIBRATION METER
MANUFACTURER	:	INSTANTEL
MODEL / TYPE	:	721A2601/721A3301
SERIAL NO.	:	UM19244/UM19244
CLID. NO.	:	252402113
JOB CONTROL NO.	:	240919100992
CALIBRATION SERVICE	:	☑ IN-LABORATORY ☐ ON-SITE

CUSTOMER : TNP ENVIRONMENT CO., LTD.
332/173 MOO 3 TAMBON BANG RAK PHATTANA,
AMPHOE BANG BUA THONG, NONTHABURI 11110

DATE OF RECEIVED : 19 September 2024 DATE OF ISSUED : 28 September 2024

The report of calibration shall not be reproduced except in full without approval of the Calibration Laboratory Co., Ltd.

Calibrated By : [redacted]

Approved By : [redacted]

28 September 2024

This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to the International System of Units (SI)

Certificate No. Q24100992

F3-011-05/12-23

@clccalibration

CALIBRATION LABORATORY CO., LTD.
2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com

CLC Accredited ISO/IEC 17025

ilac-MRA

ANAB ANSI National Accreditation Board ACCREDITED ISO/IEC 17025 CALIBRATION AND DIMENSIONAL MEASUREMENT ACDM-2814

REPORT OF CALIBRATION

FOR

NOMENCLATURE	:	**VIBRATION METER**
MANUFACTURER	:	**INSTANTEL**
MODEL / TYPE	:	**721A2601/721A3301**
SERIAL NO.	:	**UM19244/UM19244**
DATE OF CALIBRATION	:	**26 September 2024**

ENVIRONMENT CONDITIONS :

Temperature : (23 ± 2) °C **Relative Humidity :** (55 ± 15) %RH

PROCEDURE USED :

This instrument was calibrated under procedure No. **CLC-CPEE-08** based on **ISO 16063-21** as calibration guideline.

The calibration was performed by using Digital Multimeter, Programmable Timer/Counter, Accelerometer and Measuring Amplifier which maintained by the Calibration Laboratory Co., Ltd.

REFERENCE STANDARD USED :

1. Digital Multimeter, Hewlett Packard Model 34401A S/N. 3146A75935.
2. Programmable Timer/Counter, Philips Model PM6680B S/N. SM607101.
3. Accelerometer with Measuring Amplifier, Bruel & Kjaer Model 8305, 2626 S/N. 705491, 1741406.

TRACEABILITY :

1. The measurements are traceable to International System of Units (SI), through National Institute of Metrology (Thailand) Certificate No. EE-0130-23, Due Date 29 November 2024.
2. The measurements are traceable to International System of Units (SI), through Aeronautical Radio of Thailand Ltd. Certificate No. 07-0050/24 , Due Date 13 May 2025 .
3. The measurements are traceable to International System of Units (SI), through National Institute of Metrology (Thailand) Certificate No. AV-0053-23, Due Date 12 October 2024.

UNCERTAINTY :

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor $k = 2{,}00$ which for a normal distribution corresponds to a coverage probability of approximately 95 %. It has been evaluated according to the "Evaluation of the Uncertainty of Measurement in Calibration (EA-4/02 M:2022)"

@clccalibration

CONDITION OF CALIBRATION ITEM : RECEIVED IN GOOD OPERATIONAL CONDITION

MEASUREMENT RESULTS : (X) without adjustment ( ) adjustment

CALIBRATION DATA

1. VELOCITY RESULT

Test point		Mode	STD Reading	DUC Reading	Correction	Uncertainty
(mm/s)	(frequency)		(mm/s)	(mm/s)	(mm/s)	± (% of rdg.)
10	80 Hz	peak	10.000	10.089	-0.089	1.6
20	80 Hz		20.000	20.156	-0.156	1.1
30	80 Hz		30.000	30.196	-0.196	1.0
40	80 Hz		40.000	40.256	-0.256	0.9
50	80 Hz		50.000	50.311	-0.311	0.9

Note. The Scope of Accredited ANAB Certificate No. ACDM-2814 Version 012 Page 2 of 67

CALIBRATION LABORATORY CO., LTD.
2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com

CLC Accredited ISO/IEC 17025

ANAB ANSI National Accreditation Board ACCREDITED ISO/IEC 17025 CALIBRATION AND DIMENSIONAL MEASUREMENT ACDM-2814

CALIBRATION DATA

*2. FREQUENCY RESULT

STD Applied (Hz)	DUC Reading (Hz)	Correction (Hz)	Uncertainty ± (Hz)
50	50	0	0.8
80	80	0	0.8
100	100	0	0.8

Note. * means Calibrations marked " Not ANAB Accredited " in this Certificate have been included for completeness.

This report is valid for the above stated instrument/s only.

End of Certificate

METROLOGY SYSTEM (THAILAND) CO.,LTD.

ID LINE : IEC17025

69/29 Moo 1 Klongsi Klongluang Pathumthani 12120 (Thailand) Tel: (662) 193-2220 5 คู่สาย www.สอบเทียบเครื่องมือวัด.com

Certificate of Calibration

Certificate Number : SPR24050187-1

Customer : TNP ENVIRONMENT CO.,LTD.
332/173 Moo.3, Bang Rak Phatthana, Bang Bua Thong, Nonthaburi 11110

Equipment Name	: Autoclave		
Manufacturer	: BIOBASE		
Model	: BKQ-Z50I		
Serial Number	: BKQ-Z50I23055014		
ID. Number	: TNP.LAB.56		
Environmental Conditions			
Ambient Temperature	: 25 °C ± 10 °C	Received Date	: 11 May 2024
Relative Humidity	: 60 % ± 20 %	Calibration Date	: 16 May 2024
Location of Calibration	: On-Site	Recommend Due Date	: 16 May 2025
Calibration Procedure	: SP-CPT-04-04	Date of Issue	: 17 May 2024

Method of Calibration

This certifies that the above instrument was calibrated in compliance with the calibration system requirement of ISO/IEC 17025:2017 in accordance with reference procedure. Standards used to perform this calibration are certified by to NIST or equivalent, National metrology institute, Natural physical constants, consensus standards. The result reported herein apply only to the calibration of the item described above as received.Our decision rule is to contact the customer if the item pass and fail calibration when the results include the uncertainties and the customer must determine if the results meets their needs.

The calibration certificate shall not be reproduced except in full,without written approval of SP Metrology System (Thailand).

Calibrated by : [redacted]

Approved by : [redacted]

METROLOGY SYSTEM (THAILAND) CO.,LTD.

ID LINE : IEC17025

69/29 Moo 1 Klongsi Klongluang Pathumthani 12120 (Thailand) Tel: (662) 193-2220 5 สายงาน www.สอบเทียบเครื่องมือวัด.com

Calibration Report

Certificate Number : SPR24050187-1

Reference Standards

Equipment Name	Model	Serial No.	Certificate No.	Due. Date
Data Acquisition/Switch Unit	34970A	MY44074688	SPR24010142-25	11 Jan 2025

Traceability

This certification is traceable to the International System of Unit maintained at :

SP Metrology - SP Metrology system (Thailand) Co.Ltd.


METROLOGY SYSTEM (THAILAND) CO.,LTD.

ID LINE : IEC17025

69/29 Moo 1 Klongsi Klongluang Pathumthani 12120 (Thailand) Tel: (662) 193-2220 5 คู่สาย www.สอบเทียบเครื่องมือวัด.com

Result of Calibration

Certificate Number : SPR24050187-1

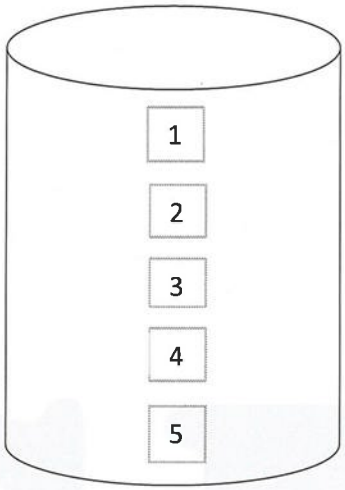

1. Temperature Accuracy in the Measurement Zone. Unit : °C

UUC Setting	Measured Temperature (°C) @ Probe No.					Uncertainty (±)
	# 1	# 2	# 3	# 4	# 5	
115.0	115.1	115.0	115.1	115.0	115.1	0.26
121.0	121.1	121.0	121.0	121.1	121.1	0.26

2. Temperature Uniformity, Stability Unit : °C

UUC Setting	UUC Reading	Temperature Stability	Temperature Uniformity
115.0	115.0	0.02	0.04
121.0	121.0	0.02	0.04

Note :

The result of calibration was found accurate as show on date and place of calibration only.

This Certificate is not certified for any commercial transaction.

Measurement Uncertainty

The reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor k = 2.00, providing a level of confidence approximately 95 %

– End of Certificate –

METROLOGY SYSTEM (THAILAND) CO.,LTD.

ID LINE : IEC17025

69/29 Moo 1 Klongsi Klongluang Pathumthani 12120 (Thailand) Tel: (662) 193-2220 5 สายต่อ www.สอบเทียบเครื่องมือวัด.com

Certificate of Calibration

Certificate Number : SPR24050187-2

Customer : TNP ENVIRONMENT CO.,LTD.
332/173 Moo.3, Bang Rak Phatthana, Bang Bua Thong, Nonthaburi 11110

Equipment Name	:	pH Meter			
Manufacturer	:	Eutech			
Model	:	pH 700			
Serial Number	:	3178920			
ID. Number	:	TNP.LAB.57			
Environmental Conditions					
Ambient Temperature	:	25 °C ± 10 °C	Received Date	:	11 May 2024
Relative Humidity	:	60 % ± 20 %	Calibration Date	:	16 May 2024
Location of Calibration	:	On-Site	Recommend Due Date	:	16 May 2025
Calibration Procedure	:	SP-CPC-04-01	Date of Issue	:	17 May 2024

Method of Calibration

This certifies that the above instrument was calibrated in compliance with the calibration system requirement of ISO/IEC 17025:2017 in accordance with reference procedure. Standards used to perform this calibration are certified by to NIST or equivalent, National metrology institute, Natural physical constants, consensus standards. The result reported herein apply only to the calibration of the item described above as received.Our decision rule is to contact the customer if the item pass and fail calibration when the results include the uncertainties and the customer must determine if the results meets their needs.

The calibration certificate shall not be reproduced except in full,without written approval of SP Metrology System (Thailand).

Calibrated by [redacted]

Approved by : [redacted]

Calibration Report

Certificate Number : SPR24050187-2

Reference Standards

Equipment Name	Model	Serial No.	Certificate No.	Due. Date
Standard pH Solution	PH016.L5	Lot No.970880	61278486	25 Apr 2025
Standard pH Solution	PH107.L5	Lot No.970881	61281486	25 Apr 2025
Standard pH Solution	PH020.L5	Lot No.970882	61297722	25 Apr 2025

Traceability

This certification is traceable to the International System of Unit maintained at :
C.P.A. Chem - ANAB#AT-1836 (ISO/IEC 17025:2017) and ANAB#AR-1835 (ISO/IEC 17034:2016)

69/29 Moo 1 Klongsi Klongluang Pathumthani 12120 (Thailand) Tel: (662) 193-2220 5 สายๆ www.สอบเทียบเครื่องมือวัด.com

METROLOGY SYSTEM (THAILAND) CO.,LTD.

ID LINE : IEC17025

69/29 Moo 1 Klongsi Klongluang Pathumthani 12120 (Thailand) Tel: (662) 193-2220 5 คู่สาย www.สอบเทียบเครื่องมือวัด.com

Result of Calibration

Certificate Number : SPR24050187-2

Range : 0 to 14 pH **Resolution :** 0.01 pH

pH Measurement @ 25 °C Unit : pH

Standard Solution	UUC Reading	Error	Uncertainty (±)
4.008	4.03	0.022	0.012
6.984	7.00	0.016	0.012
10.011	9.96	-0.051	0.013

Note :

The result of calibration was found accurate as show on date and place of calibration only. This Certificate is not certified for any commercial transaction.

Measurement Uncertainty

The reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor k = 2.00, providing a level of confidence approximately 95%.

- End of Certificate -

METROLOGY SYSTEM (THAILAND) CO.,LTD.

ID LINE : IEC17025

69/29 Moo 1 Klongsi Klongluang Pathumthani 12120 (Thailand) Tel: (662) 193-2220 5 ต่อสาย www.สอบเทียบเครื่องมือวัด.com

Certificate of Calibration

Certificate Number : SPR24050187-3

Customer : TNP ENVIRONMENT CO.,LTD.
332/173 Moo.3, Bang Rak Phatthana, Bang Bua Thong, Nonthaburi 11110

Equipment Name	: Water Bath		
Manufacturer	: Memmert		
Model	: WTB24		
Serial Number	: LD23.0297		
ID. Number	: TNP.LAB.58		
Environmental Conditions			
Ambient Temperature	: 25 °C ± 10 °C	Received Date	: 11 May 2024
Relative Humidity	: 60 % ± 20 %	Calibration Date	: 16 May 2024
Location of Calibration	: On-Site	Recommend Due Date	: 16 May 2025
Calibration Procedure	: SP-CPT-04-04	Date of Issue	: 17 May 2024

Method of Calibration

This certifies that the above instrument was calibrated in compliance with the calibration system requirement of ISO/IEC 17025:2017 in accordance with reference procedure. Standards used to perform this calibration are certified by to NIST or equivalent, National metrology institute, Natural physical constants, consensus standards. The result reported herein apply only to the calibration of the item described above as received.Our decision rule is to contact the customer if the item pass and fail calibration when the results include the uncertainties and the customer must determine if the results meets their needs.

The calibration certificate shall not be reproduced except in full,without written approval of SP Metrology System (Thailand).

Calibrated by : [redacted]

Approved by : [redacted]

METROLOGY SYSTEM (THAILAND) CO.,LTD.

ID LINE : IEC17025

69/29 Moo 1 Klongsi Klongluang Pathumthani 12120 (Thailand) Tel: (662) 193-2220 5 สายๆ www.สอบเทียบเครื่องมือวัด.com

Calibration Report

Certificate Number : SPR24050187-3

Reference Standards

Equipment Name	Model	Serial No.	Certificate No.	Due. Date
Data Acquisition/Switch Unit	34970A	MY44074688	SPR24010142-25	11 Jan 2025

Traceability

This certification is traceable to the International System of Unit maintained at :

SP Metrology - SP Metrology system (Thailand) Co.Ltd.


METROLOGY SYSTEM (THAILAND) CO.,LTD.

ID LINE : IEC17025

69/29 Moo 1 Klongsi Klongluang Pathumthani 12120 (Thailand) Tel: (662) 193-2220 5 ต่อสาย www.สอบเทียบเครื่องมือวัด.com

Result of Calibration

Certificate Number : SPR24050187-3

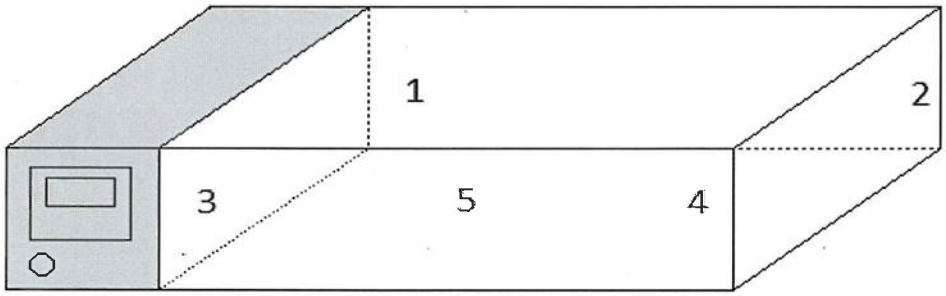

1. Temperature Accuracy in the Measurement Zone.

Unit : °C

UUC Setting	Measured Temperature (°C) @ Probe No.					Uncertainty (±)
	# 1	# 2	# 3	# 4	# 5	
44.5	44.54	44.44	44.50	44.50	44.47	0.19

2. Temperature Uniformity, Stability

Unit : °C

UUC Setting	UUC Reading	Temperature Stability	Temperature Uniformity
44.5	44.5	0.07	0.20

Note :

The result of calibration was found accurate as show on date and place of calibration only. This Certificate is not certified for any commercial transaction.

Measurement Uncertainty

The reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor k = 2.00, providing a level of confidence approximately 95 %

- End of Certificate -

METROLOGY SYSTEM (THAILAND) CO.,LTD.

ID LINE : IEC17025

69/29 Moo 1 Klongsi Klongluang Pathumthani 12120 (Thailand) Tel: (662) 193-2220 5 สายต่อ www.สอบเทียบเครื่องมือวัด.com

Certificate of Calibration

Certificate Number : SPR24050187-4

Customer : TNP ENVIRONMENT CO.,LTD.
332/173 Moo.3, Bang Rak Phatthana, Bang Bua Thong, Nonthaburi 11110

Equipment Name : Incubator

Manufacturer : BIOBASE

Model : BJPX-M100B

Serial Number : BJPXM1002301016

ID. Number : TNP.LAB.59

Environmental Conditions

Ambient Temperature : 25 °C ± 10 °C

Relative Humidity : 60 % ± 20 %

Location of Calibration : On-Site

Calibration Procedure : SP-CPT-04-01

Received Date : 11 May 2024

Calibration Date : 16 May 2024

Recommend Due Date : 16 May 2025

Date of Issue : 17 May 2024

Method of Calibration

This certifies that the above instrument was calibrated in compliance with the calibration system requirement of ISO/IEC 17025:2017 in accordance with reference procedure. Standards used to perform this calibration are certified by to NIST or equivalent, National metrology institute, Natural physical constants, consensus standards. The result reported herein apply only to the calibration of the item described above as received.Our decision rule is to contact the customer if the item pass and fail calibration when the results include the uncertainties and the customer must determine if the results meets their needs.

The calibration certificate shall not be reproduced except in full,without written approval of SP Metrology System (Thailand).

Calibrated by : [redacted]

Approved by : [redacted]

Calibration Report

Certificate Number : SPR24050187-4

Reference Standards

Equipment Name	Model	Serial No.	Certificate No.	Due. Date
Data Acquisition/Switch Unit	34970A	MY44074688	SPR24010142-25	11 Jan 2025

Traceability

This certification is traceable to the International System of Unit maintained at :

SP Metrology - SP Metrology system (Thailand) Co.Ltd.

69/29 Moo 1 Klongsi Klongluang Pathumthani 12120 (Thailand) Tel: (662) 193-2220 5 คู่สาย www.สอบเทียบเครื่องมือวัด.com


METROLOGY SYSTEM (THAILAND) CO.,LTD.

ID LINE : IEC17025

69/29 Moo 1 Klongsi Klongluang Pathumthani 12120 (Thailand) Tel: (662) 193-2220 5 คู่สาย www.สอบเทียบเครื่องมือวัด.com

Result of Calibration

Certificate Number : SPR24050187-4

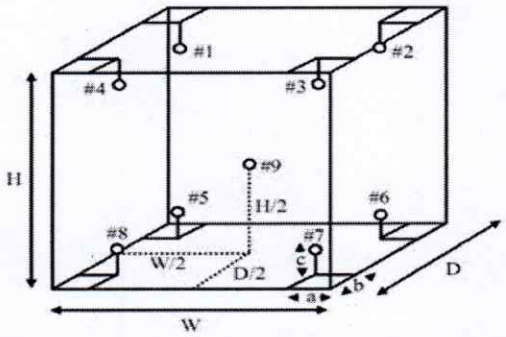

Temperature Accuracy in the Measurement Zone.

Unit : °C

UUC Setting	Measured Temperature (°C) @ Probe No. (Probe No. 9 is REF.)									Uncertainty (±)
	# 1	# 2	# 3	# 4	# 5	# 6	# 7	# 8	# 9	
35.0	35.20	35.17	35.26	35.22	35.28	35.18	35.24	35.22	35.28	0.19
37.0	37.16	37.24	37.24	37.20	37.23	37.27	37.19	37.23	37.28	0.19
41.5	41.68	41.72	41.77	41.72	41.67	41.74	41.74	41.75	41.79	0.19
42.0	42.22	42.25	42.18	42.28	42.30	42.32	42.27	42.31	42.33	0.19

Temperature Uniformity, Stability,Overall Variation

Unit : °C

UUC Setting	UUC Reading	Temperature Stability	Temperature Uniformity	Overall Variation
35.0	35.0	0.09	0.30	0.30
37.0	37.0	0.11	0.32	0.33
41.5	41.5	0.09	0.26	0.28
42.0	42.0	0.10	0.31	0.36

Note :

The result of calibration was found accurate as show on date and place of calibration only.

This Certificate is not certified for any commercial transaction.

Measurement Uncertainty

The reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor k = 2, providing a level of confidence approximately 95 %

- End of Certificate -

ENTECH
Where Solutions Begin

Calibration Certificate

NSC-TISI-TIS 17025
CALIBRATION 0157

Certificate No. T/O 670044
Date of issue : 15-Mar-2024

Equipment Description	:	Incubator
Equipment Model	:	SMART i250-DS
Equipment Serial No.	:	0410-0121-0003
I.D. No. or Control No.	:	-
Manufacturer	:	Entech Industrial Solution Co.,Ltd.
Customer Name	:	TNP ENVIRONMENT.CO.,LTD
Customer Address	:	332/173 Bang Rak Phatthana Subdistrict, Bang Bua Thong District, Nonthaburi 11110
Total pages of certificate	:	2 pages
Instrument Receiving Date	:	14-Mar-2024
Receiving No.	:	O-240062
Environmental Conditions	:	All of the measurement were carried out in the working area Temperature : (25 ± 15) °C Humidity : (55 ± 30) % RH Voltage : (220 ± 22) VAC
Calibration Place	:	(TNP Lab) 332/173 Bang Rak Phatthana Subdistrict,Bang Bua Thong District, Nonthaburi 11110 Thailand
Calibration Procedure No.	:	This instrument was calibrated by comparison of reference radiation source standard according to calibration work instruction no WI-CL-18-C

The calibration certificate expended uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k, which for a normal distribution corresponds to a coverage probability of approximately 95%

The standard uncertainty of measurement has been determined in accordance with M 3003
The expression uncertainty and confidence in measurement.

This certificate is applied only to item under test environmental condition.

This calibration certificate may not be reproduced other than in full except with the permission of the issuing laboratory. Calibration certificates without signature and seal are not valid and The results relate only to the items tested/calibrated .

This calibration certificate documents are traceability to national standards, which realize the unit of measurement according to the International system of units (SI).

Date of Calibration : 14-Mar-2024

[redacted]

Entech Industrial Solution Co.,Ltd.
17/121 Soi Ngamwongwan 47 Yaek 48, Toongsonghong, Laksi, Bangkok 10210 THAILAND Tel. 0-2779-8888 Calibration@entech.co.th
Tax ID : 0105536035591 www.entech.co.th

ENTECH
Where Solutions Begin

Calibration Certificate

NSC-TISI-TIS 17025
CALIBRATION 0157

Certificate No. : T/O 670044


The Reference Standard Instrument :-

Instrument	Model	Serial No.	Cert No.	Due date
1) Data logger with RTD Probe	Agilent 34972A	MY49017365	PSL-T 0484-3/67	19-Feb-2025

Measured room conditions

Temperature :	Minimum:	23.6 °C	Maximum:	24.2 °C
Humidity :	Minimum:	48.5 %RH	Maximum:	56.9 %RH
Voltage :	Minimum:	220.1 VAC	Maximum:	223.4 VAC
Fresh Air Setting:	off			

Sensor Position :

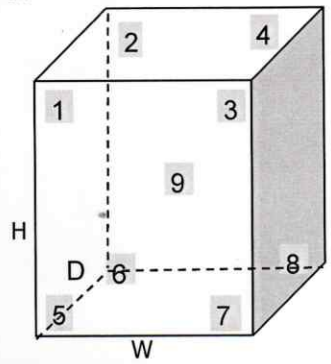

Working Space of chamber :

(Inside Dimensions) W x D x H : 500 mm x 480 mm x 1100 mm

Sensor Installation Details :

- Sensor Number 1 to 8 installed approximately 50 mm From each wall.
- Sensor Number 9 installed approximately geometric of the chamber.

Results : The measurement results of the calibration were reported in the table below.

(*) Without adjustment ( ) After adjustment

UUC* Setting	UUC* Reading	Temperature Reading oF Standard Sensor								
		Sensor Position								
(°C)	(°C)	1	2	3	4	5	6	7	8	9
20.0	20.0	20.50	19.56	20.31	20.34	20.41	20.28	20.18	20.21	20.30

UUC* Setting	UUC* Reading	Temperature Uniformity	Temperature Stability	Overall Variation	Uncertainty of Measurement	Coverage Factor
(°C)	(°C)	(°C)	(± °C)	(°C)	(± °C)	K
20.0	20.0	0.88	0.37	1.33	0.51	2

UUC* = Unit Under Calibration

Remark :-

- Temperature reading of Standard Sensors shown in the table were taken from the average of Standard reading at each position.
- Temperature Uniformity was calculated from the difference between the maximum and minimum of actual temperature reading from all reference sensors at the same time.
- Temperature Stability was calculated from the maximum stability of nine positions, and formula of Stability is [(Maximum Temperature Value - Minimum Temperature Value) /2]
- Overall Variation was calculated from the difference between the maximum and minimum measured temperature throughout observation time.

End of Report

Entech Industrial Solution Co.,Ltd.
17/121 Soi Ngamwongwan 47 Yaek 48, Toongsonghong, Laksi, Bangkok 10210 THAILAND Tel. 0-2779-8888 Calibration@entech.co.th
Tax ID : 0105536035591 www.entech.co.th

THAI CALIBRATION SERVICES CO., LTD.
19/8 Moo 9 Soi Raiking 30 Puttamonton 5 Rd., Sampran, Nakornpatom 73210
Tel. 0-3439-7682-5 Fax: 0-3439-7687
www.thaical.com E-mail : sale@thaicalibration.com, lab@thaicalibration.com

NSC-TISI-TIS 17025
CALIBRATION 0189

CALIBRATION CERTIFICATE

Certificate No.S2406450S

Customer : TNP ENVIRONMENT CO., LTD.
332/173 Moo 3 Tambon Bang Rak Phatthana,
Amphoe Bang Bua Thong, Nonthaburi 11110

Equipment : Non-automatic weighing instrument (Electronic instrument)

Manufacturer :	Sartorius	**Order No. :**	67S2626-1
Model :	SECURA224-1S	**Ambient temperature :**	(27.3 ± 5.0) °C
Accuracy class :	-	**Relative humidity :**	(33.0 ± 10.0) %
Capacity :	220 g	**Received date :**	17-Jun-2024
Resolution :	0.0001 g	**Date of calibration :**	17-Jun-2024
Serial No. :	0041305301	**Date of issue :**	19-Jun-2024
ID No. :	TNP.LAB.31	**Condition of the balance :**	Good working conditions
Place of calibration :	ห้อง LAB		

Calibration method

This instrument was calibrated according to the EURAMET Calibration Guide No. 18.

Condition of reference standard weight

Instrument	Nominal value	Serial No.	Certificate No.	Due-date	Density (kg/m^3)
1 Standard weight set	1 mg to 2 kg	15885+15849	M2310001S	7-Oct-2024	7950

Traceability of the reference standard weight

This certificate is traceable to SI unit through Mass Calibration Laboratory Thai Calibration Services Co., Ltd., NSC-ONSC accredited no. Calibration 0189.

Calibrated By [redacted]

**This calibration certificate may not be reproduced other than in full,
except with the prior written approval of the head of TCS calibration laboratory.**

NO. 16329

THAI CALIBRATION SERVICES CO., LTD.
19/8 Moo 9 Soi Raiking 30 Puttamonton 5 Rd., Sampran, Nakornpatom 73210
Tel. 0-3439-7682-5 Fax: 0-3439-7687
www.thaical.com E-mail : sale@thaicalibration.com, lab@thaicalibration.com

NSC-TISI-TIS 17025
CALIBRATION 0189

CALIBRATION CERTIFICATE


Certificate No.S2406450S

The repeatability of indication

Nominal Value (g)	Standard Deviation of reading (g)	Maximum difference between suscessive reading (g)	n
200	0.00000	0.0000	5

The effect of eccentric application of a load on the indication (test load : 100 g)

Position	Balance Reading (g)
Point 1	100.0000
Point 2	99.9999
Point 3	100.0000
Point 4	100.0000
Point 5	100.0000
Eccentric Value	0.0001



The error of indication

Nominal Value (g)	Value of Reference Standard Weight (g)	Balance Reading (g)	Correction (g)	Uncertainty (±) (g)	*k*
Unload	0.0000	0.0000	0.0000	0.000082	2.00
0.1	0.1000	0.1000	0.0000	0.000083	2.00
0.5	0.5000	0.5000	0.0000	0.000084	2.00
1	1.0000	1.0000	0.0000	0.000085	2.00
5	5.0000	5.0001	-0.0001	0.000089	2.00
10	10.0000	10.0000	0.0000	0.000093	2.00
20	20.0000	20.0000	0.0000	0.00010	2.00
50	50.0000	50.0000	0.0000	0.00012	2.00
100	99.9999	100.0000	-0.0001	0.00015	2.00
200	199.9999	199.9999	0.0000	0.00026	2.00

Remark : Adjustment, External weight nominal value 200 g, Standard weight of Lab

Uncertainty of measurement

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor (*k*), which for a normal distribution corresponds to a coverage probability of approximately 95% (confidence level).

This report will certify of the calibrated equipment only.

--End--

NO. 16330

ENTECH
Where Solutions Begin

Calibration Certificate

NSC-TISI-TIS 17025
CALIBRATION 0157

Certificate no: H/T 670338
Date of issue : 21-Mar-24

Instrument description	:	Thermo-Hygrometer
Instrument model	:	Extech 445815
Instrument serial no.	:	PONPE5899554
ID no. or control no.	:	TNP.LAB.21
Manufacturer	:	Extech Instruments
Probe description	:	-
Probe model	:	-
Probe serial	:	-
Customer name	:	TNP ENVIRONMENT CO.,LTD.
Customer address	:	332/173 Moo 3 Tambon Bang Rak Phatthana, Amphoe Bang Bua Thong, Nonthaburi 11110
Total pages of certificate	:	2 Pages
Receiving no.	:	L-241004-1
Receiving date.	:	08-Mar-24
Parameter of calibration	:	Temperature Calibration
Condition of UUC.	:	Used
Ambient condition	:	All of the Measurement were carried out the stabilized laboratory Temperature : 23 ±5 °C Humidity : 55 ± 15 %RH
Calibration place	:	17/121 Soi Ngamwongwan 47 Yaek 48, Toongsonghong, Laksi, Bangkok 10210
Calibration procedure no.	:	This instrument was calibrated by comparison of indication with the Standard Thermo- hygrometer according to calibration Work Instruction no .WI-CL-11-C

The calibration certificate expanded uncertainty of measurement is stated as the standard uncertainty of measurent Multiplied by coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

This certificate is applied only to item under test Environmental condition.

This Calibration Certificate may not be reporduced other than in full except with the permission of the issuing laboratory. Calibration certificates without signature and seal not valid.

This calibration certificate documents are tracebility to national standards, which realize measurement according to the International System of Units (SI).

Date of calibration : 20-Mar-24

[redacted]

Entech Industrial Solution Co.,Ltd.
17/121 Soi Ngamwongwan 47 Yaek 48, Toongsonghong, Laksi, Bangkok 10210 THAILAND Tel. 0-2779-8888 Calibration@entech.co.th
Tax ID : 0105536035591 www.entech.co.th

Certificate no: H/T 670338

Standard refereces

Standard	Reference No.	Vendor	Due Date
ARALAB 300ECP,Fitoclima	S2023070040-001	MIT	07-Jul-24
Thermo HygroPalm HP 23-A	SG-H-00579/66	Success Gateway	16-Aug-24

Measured room conditions

Temperature : 22.1 **°C** **Humidity :** 55.9 **%RH** **Pressure :** 1019.3 **mbar**

Calibration results (Without Adjustment) **Reference temperature :** - **°C**

Parameter of standard	Standard values	Mean of UUC.	Error	Uncertainty (±)
Temperature (°C)	19.97	20.1	0.13	0.50
Temperature (°C)	25.02	25.2	0.18	0.50
Temperature (°C)	29.99	30.2	0.21	0.50

Remark : -

End of Report

Entech Industrial Solution Co.,Ltd.
17/121 Soi Ngamwongwan 47 Yaek 48, Toongsonghong, Laksi, Bangkok 10210 THAILAND Tel. 0-2779-8888 Calibration@entech.co.th
Tax ID : 0105536035591 www.entech.co.th

THAI CALIBRATION SERVICES CO., LTD.
19/8 Moo 9 Soi Raiking 30 Puttamonton 5 Rd., Sampran, Nakornpatom 73210
Tel. 0-3439-7682-5 Fax: 0-3439-7687
www.thaical.com E-mail : sale@thaicalibration.com, lab@thaicalibration.com

NSC-TISI-TIS 17025
CALIBRATION 0189

CALIBRATION CERTIFICATE

Certificate No.S2406451S

Customer : TNP ENVIRONMENT CO., LTD.
332/173 Moo 3 Tambon Bang Rak Phatthana,
Amphoe Bang Bua Thong, Nonthaburi 11110

Equipment : Non-automatic weighing instrument (Electronic instrument)

Manufacturer :	Shimadzu	**Order No. :**	67S2626-2
Model :	AP225WD	**Ambient temperature :**	(27.2 ± 5.0) °C
Accuracy class :	-	**Relative humidity :**	(34.0 ± 10.0) %
Capacity :	102 g / 220 g	**Received date :**	17-Jun-2024
Resolution :	0.00001 g / 0.0001 g	**Date of calibration :**	17-Jun-2024
Serial No. :	D316301848	**Date of issue :**	19-Jun-2024
ID No. :	TNP.LAB.30	**Condition of the balance :**	Good working conditions
Place of calibration :	ห้อง LAB		

Calibration method

This instrument was calibrated according to the EURAMET Calibration Guide No. 18.

Condition of reference standard weight

Instrument	Nominal value	Serial No.	Certificate No.	Due-date	Density (kg/m^3)
1 Standard weight set	1 mg to 2 kg	15885+15849	M2310001S	7-Oct-2024	7950

Traceability of the reference standard weight

This certificate is traceable to SI unit through Mass Calibration Laboratory Thai Calibration Services Co., Ltd., NSC-ONSC accredited no. Calibration 0189.

Calibrated By S[redacted]

**This calibration certificate may not be reproduced other than in full,
except with the prior written approval of the head of TCS calibration laboratory.**

NO. 16331

THAI CALIBRATION SERVICES CO., LTD.
19/8 Moo 9 Soi Raiking 30 Puttamonton 5 Rd., Sampran, Nakornpatom 73210
Tel. 0-3439-7682-5 Fax: 0-3439-7687
www.thaical.com E-mail : sale@thaicalibration.com, lab@thaicalibration.com

NSC-TISI-TIS 17025
CALIBRATION 0189

CALIBRATION CERTIFICATE


Certificate No.S2406451S

The repeatability of indication

Nominal Value (g)	Standard Deviation of reading (g)	Maximum difference between sucessive reading (g)	n
100	0.000009	0.00002	5
200	0.00005	0.0001	5

The effect of eccentric application of a load on the indication (test load : 100 g)

Position	Balance Reading (g)
Point 1	100.00000
Point 2	100.00002
Point 3	100.00000
Point 4	99.99994
Point 5	99.99995
Eccentric Value	0.00006



The error of indication

Nominal Value (g)	Value of Reference Standard Weight (g)	Balance Reading (g)	Correction (g)	Uncertainty (±) (g)	*k*
Unload	0.00000	0.00000	0.00000	0.000027	2.65
0.1	0.10000	0.10003	-0.00003	0.000026	2.28
0.5	0.50000	0.50003	-0.00003	0.000029	2.15
1	1.00000	1.00004	-0.00004	0.000031	2.10
5	4.99998	5.00001	-0.00003	0.000041	2.03
10	9.99999	10.00002	-0.00003	0.000047	2.00
20	20.00000	19.99998	+0.00002	0.000060	2.00
50	50.00001	50.00003	-0.00002	0.000074	2.00
100	99.99995	100.00000	-0.00005	0.00012	2.00
200	199.9999	200.0000	-0.0001	0.00026	2.00

Remark : Adjustment, External weight nominal value 100 g, Standard weight of Lab

Uncertainty of measurement

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor (*k*), which for a normal distribution corresponds to a coverage probability of approximately 95% (confidence level).

This report will certify of the calibrated equipment only.

--End--

THAI CALIBRATION SERVICES CO., LTD.
19/8 Moo 9 Soi Raiking 30 Puttamonton 5 Rd., Sampran, Nakornpatom 73210
Tel. 0-3439-7682-5 Fax: 0-3439-7687
www.thaical.com E-mail : sale@thaicalibration.com, lab@thaicalibration.com

NSC-TISI-TIS 17025
CALIBRATION 0189

CALIBRATION CERTIFICATE

Certificate No.S2406450S

Customer : TNP ENVIRONMENT CO., LTD.
332/173 Moo 3 Tambon Bang Rak Phatthana,
Amphoe Bang Bua Thong, Nonthaburi 11110

Equipment : Non-automatic weighing instrument (Electronic instrument)

Manufacturer :	Sartorius	**Order No. :**	67S2626-1
Model :	SECURA224-1S	**Ambient temperature :**	(27.3 ± 5.0) °C
Accuracy class :	-	**Relative humidity :**	(33.0 ± 10.0) %
Capacity :	220 g	**Received date :**	17-Jun-2024
Resolution :	0.0001 g	**Date of calibration :**	17-Jun-2024
Serial No. :	0041305301	**Date of issue :**	19-Jun-2024
ID No. :	TNP.LAB.31	**Condition of the balance :**	Good working conditions
Place of calibration :	ห้อง LAB		

Calibration method

This instrument was calibrated according to the EURAMET Calibration Guide No. 18.

Condition of reference standard weight

Instrument	Nominal value	Serial No.	Certificate No.	Due-date	Density (kg/m^3)
1 Standard weight set	1 mg to 2 kg	15885+15849	M2310001S	7-Oct-2024	7950

Traceability of the reference standard weight

This certificate is traceable to SI unit through Mass Calibration Laboratory Thai Calibration Services Co., Ltd., NSC-ONSC accredited no. Calibration 0189.

Calibrated By Sa[redacted]

This cal[redacted]
except with the prior written approval of the head of TCS calibration laboratory.

NO. 16329

THAI CALIBRATION SERVICES CO., LTD.
19/8 Moo 9 Soi Raiking 30 Puttamonton 5 Rd., Sampran, Nakornpatom 73210
Tel. 0-3439-7682-5 Fax: 0-3439-7687
www.thaical.com E-mail : sale@thaicalibration.com, lab@thaicalibration.com

NSC-TISI-TIS 17025
CALIBRATION 0189

CALIBRATION CERTIFICATE


Certificate No.S2406450S

The repeatability of indication

Nominal Value (g)	Standard Deviation of reading (g)	Maximum difference between sucessive reading (g)	n
200	0.00000	0.0000	5

The effect of eccentric application of a load on the indication (test load : 100 g)

Position	Balance Reading (g)
Point 1	100.0000
Point 2	99.9999
Point 3	100.0000
Point 4	100.0000
Point 5	100.0000
Eccentric Value	0.0001



The error of indication

Nominal Value (g)	Value of Reference Standard Weight (g)	Balance Reading (g)	Correction (g)	Uncertainty (±) (g)	*k*
Unload	0.0000	0.0000	0.0000	0.000082	2.00
0.1	0.1000	0.1000	0.0000	0.000083	2.00
0.5	0.5000	0.5000	0.0000	0.000084	2.00
1	1.0000	1.0000	0.0000	0.000085	2.00
5	5.0000	5.0001	-0.0001	0.000089	2.00
10	10.0000	10.0000	0.0000	0.000093	2.00
20	20.0000	20.0000	0.0000	0.00010	2.00
50	50.0000	50.0000	0.0000	0.00012	2.00
100	99.9999	100.0000	-0.0001	0.00015	2.00
200	199.9999	199.9999	0.0000	0.00026	2.00

Remark : Adjustment, External weight nominal value 200 g, Standard weight of Lab

Uncertainty of measurement

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor (*k*), which for a normal distribution corresponds to a coverage probability of approximately 95% (confidence level).

This report will certify of the calibrated equipment only.

--End--

NO. 16330

Harikul Science Co.,Ltd.
694 Soi Ratchadanivet 24, Pracharatbamphen,
Samsaennok, Huaikhwang, Bangkok 10310
Tel: 0-2274-2456 Fax: 0-2274-2443
Email: info@harikul.com www.harikul.com

CERT.No.: HS-V032E

Certificate of Calibration

Calibration Date : 30 May 24

Submitted by : TNP ENVIRONMENT COMPANY LIMITED.
332/173 Moo. 3, Tambon Bang Rak Phatthana,
Amphoe Bang Bua Thong, Nonthaburi 11110

Avg Room Temp : 20 °C
Avg Water Temp : 20 °C
Air Pressure : 757.00 mmH
Salinity : 0 ppt

Model : YSI 4010-2W
S/N : 22051520
Probe : YSI 4100 BOD
S/N : 22C102711
ID NO. :
Air Temp ref : S/N. F8065C26
Barometric ref : S/N. F8065C26
Water Temp ref : S/N. 11431

Technician : Kittipong M.

Calibration Details

Calibration Point	100% air sat. (@20 °C, DO = 9.09 mg/l)	(status)		(status)
Measurement 1 (mg/l)	9.06	(PASS)	-	-
Measurement 2 (mg/l)	9.05	(PASS)	-	-
Measurement 3 (mg/l)	9.04	(PASS)	-	-
Measurement 4 (mg/l)	9.04	(PASS)	-	-
Measurement 5 (mg/l)	9.03	(PASS)	-	-
Measurement 6 (mg/l)	9.03	(PASS)	-	-
Measurement 7 (mg/l)	9.03	(PASS)	-	-
Measurement 8 (mg/l)	9.02	(PASS)	-	-
Measurement 9 (mg/l)	9.02	(PASS)		-
Measurement 10 (mg/l)	9.02	(PASS)	-	-
Mean Measurement	9.03	mg/l	-	-
Inaccuracy	0.06	mg/l	-	-
Overall Status	(PASS)			

Manufacturer Specification

Accuracy = +/- 0.2 mg/l

1) This certificate is issued based on the result that are found as shown on date and place of test only.
2) The calibration procedure followed in accordance with Harikul Science Co., Ltd.
3) This result shall not be used for advertising purpose.

[redacted]

[redacted]

Harikul Science Co.,Ltd.
694 Soi Ratchadanivet 24, Pracharatbamphen,
Samsaennok, Huaikhwang, Bangkok 10310
Tel: 0-2274-2456 Fax: 0-2274-2443
Email: info@harikul.com www.harikul.com

Certificate of Calibration

CERT.No.: HS-V022D

Calibration Date : 10 Apr 24

Submitted by : TNP ENVIRONMENT COMPANY LIMITED
332/173 Moo.3, Tambon Bang Rak Phatthana,
Amphoe Bang Bua Thong, Nonthaburi 11110

Avg Room Temp : 20 °C
Avg Water Temp : 20 °C
Air Pressure : 761.00 mmHg
Salinity : 0 ppt

Model : HI 5421
S/N : 07210004101
Probe : HI 76408W
S/N : KC1N32W9P
ID NO. :
Air Temp ref : S/N. F8065C26
Barometric ref : S/N. F8065C26
Water Temp ref : S/N. 11430

Technician : Kittipong M.

Calibration Details

Calibration Point	100% air sat. (@20 °C, DO = 9.08 mg/l)	(status)		(status)
Measurement 1 (mg/l)	9.08	(PASS)	-	-
Measurement 2 (mg/l)	9.07	(PASS)	-	-
Measurement 3 (mg/l)	9.07	(PASS)	-	-
Measurement 4 (mg/l)	9.07	(PASS)	-	-
Measurement 5 (mg/l)	9.07	(PASS)	-	-
Measurement 6 (mg/l)	9.07	(PASS)	-	-
Measurement 7 (mg/l)	9.07	(PASS)	-	-
Measurement 8 (mg/l)	9.07	(PASS)	-	-
Measurement 9 (mg/l)	9.07	(PASS)		-
Measurement 10 (mg/l)	9.07	(PASS)	-	-
Mean Measurement	9.07	mg/l	-	-
Inaccuracy	0.01	mg/l	-	-
Overall Status	(PASS)			

Manufacturer Specification

Accuracy = +/- 0.15 mg/l

1) This certificate is issued based on the result that are found as shown on date and place of test only.
2) The calibration procedure followed in accordance with Harikul Science Co., Ltd.
3) This result shall not be used for advertising purpose.

[redacted]

[redacted]

PerkinElmer

MAINTENANCE AND IPV TEST CERTIFICATE MODEL

Avio 200

Customer :	Environment & Laboratory	**Date Tested:**	September 9, 2022
		Recommendation Recertification	
Address :	[redacted]	**Period**	12 Months
		Recertification Due:	September 9, 2023
		Date Last Certified:	January 14, 2021
User Name:		**Visit Number:**	1 of 1
Phone:		**PerkinElmer Phone:**	02-719-6420 ext 206
E - Mail :		**PerkinElmer Fax:**	02-318-5597

CONFIGURATION TESTED

MODEL	SERIAL NUMBER	SOFTWARE
Avio 200	079S16062402	

TESTED EQUIPMENT	CALIBRATION NUMBER	EXPIRATION
IPV Method		

TEST STANDARD USED	PART NUMBER	EXPIRATION DATE
Multielement Standard	N069-1579	Jun 30,2023
Instrument Cal. STD4	N930-0221	Nov 30, 2023

CUSTOMER SUPPLIED	COMMENTS	CUSTOMER INITIALS
2 % HNO3		
10 % HNO3		

PerkinElmer Ltd. 290 Soi 17 Rama 9 Road, Khwang Bangkapi, Khet Huay Kwang, Bangkok 10310, Thailand

PerkinElmer

MAINTENANCE AND IPV TEST CERTIFICATE MODEL

Avio 200

SERIAL NUMBER: 079S16062402 **DATE TESTED:** September 9, 2022

1. MECHANICAL CHECKS

A. Inspect and clean all fans and filters.	OK
B. Inspect and replace as necessary, all torch components including the RF coil.	OK
C. Inspect all tubing for sign of clacking or leaking.	OK
D. Adjust water and gas pressure regulator settings.	OK
E. Inspect and leak check pneumatics drawers.	OK
F. Clean the exterior of the instrument.	OK

2. OPTICAL CHECKS

A. Inspect and clean all optical components.	OK
B. As reqiured, check and replace all purgebfilters.	OK
C. Recheck optical alignment.	OK

3. COOLING SYSTEM CHECKS

A. Perform preventive maintenance on chiller.	OK
B. Flush out the chiller every year.	OK

4. PERFORMANCE CHECKS

A. Torch View Alignment.	OK
B. Wavelength Calibration.	OK

PerkinElmer Ltd. 290 Soi 17 Rama 9 Road, Khwang Bangkapi, Khet Huay Kwang, Bangkok 10310, Thailand

PerkinElmer

MAINTENANCE AND IPV TEST CERTIFICATE MODEL

Avio 200

SERIAL NUMBER: 079S16062402 **DATE TESTED:** September 9, 2022

PARAMETER		SPECIFICATION		FINAL VALUE	
Spectral Resolution : UV					
As 193.696 nm		≤ 0.009	nm	0.00765	nm
Ni 231.604 nm		≤ 0.011	nm	0.00885	nm
Ni 341.476 nm		≤ 0.015	nm	0.01268	nm
Spectral Resolution : VIS					
Ba 455.403 nm		≤ 0.020	nm	0.01519	nm
Precision					
Zn 206.200 nm		% RSD	≤ 1.0 %	0.58	%
Mg 280.271 nm		% RSD	≤ 1.0 %	0.17	%
Mg 285.213 nm		% RSD	≤ 1.0 %	0.18	%
Ba 455.403 nm		% RSD	≤ 1.0 %	0.22	%
Detection Limits : Axial					
Tl 190.801 nm		3(sd)		0.25	ppb
As 193.696 nm		3(sd)		1.92	ppb
Se 196.026 nm		3(sd)		0.99	
Pb 220.353 nm		3(sd)		1.24	ppb
Detection Limits : Radial					
As 193.696 nm		3(sd)		1.12	ppb
Zn 213.857 nm		3(sd)		0.06	ppb
Mn 257.610 nm		3(sd)		0.00	ppb
La 379.478 nm		3(sd)		0.09	ppb
Ba 455.403 nm		3(sd)		0.01	ppb
Ba 493.408 nm		3(sd)		0.01	ppb
BEC : Axial (IB X 1000)/(IS-IB)					
Mn 257.610 nm		≤ 30 ppb		4.50	ppb
BEC : Radial (IB X 1000)/(IS-IB)					
Mn 257.610 nm		≤ 30 ppb		5.91	ppb

PerkinElmer Ltd. 290 Soi 17 Rama 9 Road, Khwang Bangkapi, Khet Huay Kwang, Bangkok 10310, Thailand

PerkinElmer

MAINTENANCE AND IPV TEST CERTIFICATE MODEL

Avio 200

SERIAL NUMBER: 079S16062402 **DATE TESTED:** September 9, 2022

Remarks :

Commissioning follow as commissioning performance sheets.

This is to certify that the above tests have been perfomed and the configuration tested

[✔] meets

[ ] does not meet

the PerkinElmer Specifications listed on this certificate.

This certificate does not modify PerkinElmer's standard terms and condition of sale, including warranty terms.

Service Department PerkinElmer Ltd.

Customer Service Engineer: _____ ([redacted])

TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000-29 FAX. 0-2719-9484

NSC-TISI-TIS17025
CALIBRATION 0008

Cert. No.: 23TM1100

Certificate of Calibration

Equipment :	Incubator
Manufacturer :	Memmert
Model :	BM 500
Serial No. :	D593.0342
ID No. :	CHI-002
Submitted by :	Environment & Laboratory Co.,Ltd. 40 Soi Liangmueangnonthaburi 13, Talad Kwan, Mueang, Nonthaburi 11000
Location :	Room No. 204
Received Order :	12 July 2023
Calibration Date :	12 July 2023
Ambient Temperature :	(26 ± 10) °C
Relative Humidity :	(50 ± 30) %

[redacted]

Issue Date : 24 July 2023

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

Equipment : Incubator

Condition As-Received : Used Item

Reference : 2307-0094OC-4

Cert. No.: 23TM1100

Procedure Used :-

Calibration were conducted using calibration procedure CP-OT02 according to direct measurement method with Data Acquisition which connected with Resistance Temperature Detector (RTD).

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

Instrument	Serial No.	Cert. No.	Traceable	Due Date
1) Data Acquisition	MY41021843	22LM172	TPA	27 Dec 2023

2. This certificate is valid only to the item calibrated on date and place of calibration.
3. This certification is traceable to the International System of Unit.


Remark : TPA : Technology Promotion Association (Thailand - Japan)

Result of Calibration :- (*) Without Adjustment

Function of UUC* : Temperature Source

Fresh air setting : Not Available

Environment during calibration		
	Beginning	**Finished**
Temp. (°C)	22	22
REL.Humid. (%)	64	66
AC Supply (Volt)	222	221

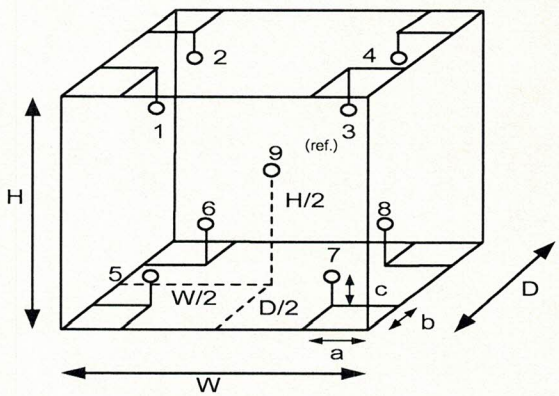

Position :	Ref. Std. ID No.:
1	18-04RTD-01
2	18-04RTD-02
3	18-04RTD-03
4	18-04RTD-04
5	18-04RTD-05
6	18-04RTD-06
7	18-04RTD-07
8	18-04RTD-08
9 (ref.)	18-04RTD-09

Probe Installation Details :

a =	5.0	cm
b =	5.0	cm
c =	5.0	cm

Dimension of Chamber :

D =	0.40	m
W =	0.56	m
H =	0.48	m
Capacity =	0.11	m^3

[redacted]

Equipment : Incubator
Condition As-Received : Used Item
Reference : 2307-0094OC-4
Result of Calibration :- (*) Without Adjustment
Function of UUC* : Temperature Source
Fresh air setting : Not Available

Cert. No.: 23TM1100

Calibration Point (°C)	UUC* Setting (°C)	UUC* Reading (°C)	Temperature stability (± °C)	Temperature uniformity (°C)	Overall Variation (°C)	Coverage Factor *k*
35.0	35.0	35.0	0.040	0.27	0.48	2

Calibration Point (°C)	Measured Temperature (°C) Position									Uncertainty (±°C)
	1	2	3	4	5	6	7	8	9 (ref.)	
35.0	35.021	34.900	35.010	35.284	34.853	34.919	34.945	34.964	35.089	0.30

Average* : The average of 30 values in each position.
Temperature stability : One-half of the greatest maximum difference of measured temperature at any one sensor.
Temperature uniformity : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.
Overall Variation : The Difference of the maximum and minimum measured temperatures throughout observation.
UUC* : Unit Under Calibration
Note : The reported uncertainty of measurement was included stability and excluded uniformity .

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor ***k***, providing a level of confidence of approximately 95 %.

-o0o-

[redacted]

TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000-29 FAX. 0-2719-9484

NSC-TISI-TIS17025
CALIBRATION 0008

Cert. No.: 23TM1273

Certificate of Calibration

Equipment :	Incubator
Manufacturer :	Envilab-Intiligent
Model :	-
Serial No. :	-
ID No. :	CHI-005
Submitted by :	Environment & Laboratory Co.,Ltd. 40 Soi Liangmueangnonthaburi 13, Talad Kwan, Mueang, Nonthaburi 11000
Location :	Room No. 204
Received Order :	24 August 2023
Calibration Date :	24 August 2023
Ambient Temperature :	(26 ± 10) °C
Relative Humidity :	(50 ± 30) %

[redacted]

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

Equipment : Incubator
Condition As-Received : Used Item
Reference : 2308-0600OC-1

Cert. No.: 23TM1273

Procedure Used :-

Calibration were conducted using calibration procedure CP-OT02 according to direct measurement method with Data Acquisition which connected with Resistance Temperature Detector (RTD).

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-


Instrument	Serial No.	Cert. No.	Traceable	Due Date
1) Data Acquisition	MY44035217	22LM170	TPA	16 Dec 2023

2. This certificate is valid only to the item calibrated on date and place of calibration.
3. This certification is traceable to the International System of Unit.

Remark : TPA : Technology Promotion Association (Thailand - Japan)

Result of Calibration :- (*) Without Adjustment
Function of UUC* : Temperature Source
Fresh air setting : Not Available

Environment during calibration		
	Beginning	Finished
Temp. (°C)	23	23
REL.Humid. (%)	50	54
AC Supply (Volt)	220	220

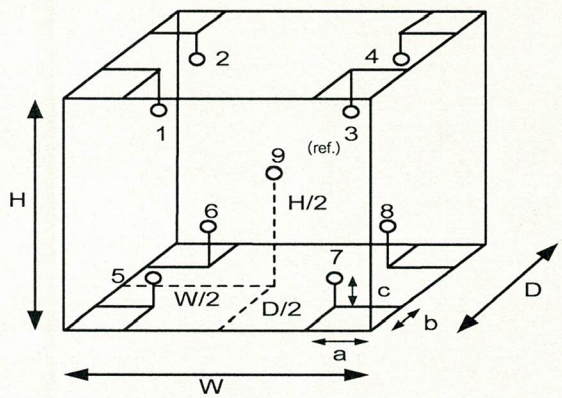

Position :	Ref. Std. ID No.:
1	18-10RTD-01
2	18-10RTD-02
3	18-10RTD-03
4	18-10RTD-04
5	18-10RTD-05
6	18-10RTD-06
7	18-10RTD-07
8	18-10RTD-08
9 (ref.)	18-10RTD-09

Probe Installation Details :

a =	5.0	cm
b =	5.0	cm
c =	5.0	cm

Dimension of Chamber :

D =	0.40	m
W =	0.70	m
H =	1.0	m
Capacity =	0.28	m^3

[redacted]

a 1176747

Equipment : Incubator
Condition As-Received : Used Item
Reference : 2308-0600OC-1
Result of Calibration :- (*) Without Adjustment
Function of UUC* : Temperature Source
Fresh air setting : Not Available

Cert. No.: 23TM1273

Calibration Point (°C)	UUC* Setting (°C)	UUC* Reading (°C)	Temperature stability (± °C)	Temperature uniformity (°C)	Overall Variation (°C)	Coverage Factor *k*
35.0	35.0	35.0	0.47	1.2	1.8	2

Calibration Point (°C)	Measured Temperature (°C) Position									Uncertainty (±°C)
	1	2	3	4	5	6	7	8	9 (ref.)	
35.0	34.805	34.737	34.701	34.435	34.724	34.783	35.228	35.604	34.816	0.71

Average* : The average of 30 values in each position.
Temperature stability : One-half of the greatest maximum difference of measured temperature at any one sensor.
Temperature uniformity : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.
Overall Variation : The Difference of the maximum and minimum measured temperatures throughout observation.
UUC* : Unit Under Calibration
Note : The reported uncertainty of measurement was included stability and excluded uniformity .

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor ***k***, providing a level of confidence of approximately 95 %.

-o0o-

[redacted]

TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000-29 FAX. 0-2719-9484

NSC-TISI-TIS17025
CALIBRATION 0008

Cert.No.: 23CHO420
Page.: 1 of 3

Certificate of Calibration

Equipment :	Spectrophotometer
Manufacturer :	Hach
Model :	DR 3900
Serial No. :	1988383
ID No. :	SPE-002
Condition As-Received:	Used Item
Received Date :	12 July 2023
Calibration Date :	12 July 2023
Reference :	2307-0094OC-11
Submitted by :	Environment & Laboratory Co.,Ltd. 40 Soi Liangmueangnonthaburi 13 Talad Kwan, Mueang, Nonthaburi 11000
Calibration Place :	Room No. 304
Ambient Temperature :	(26.7 - 26.9) °C (On-Site)
Relative Humidity :	(57.2 - 51.2) % (On-Site)
Calibration Procedure :	In - house method : CP-OCH4 based on ASTM E 275-01

[redacted]

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

A 0056486

Condition of calibration result

1. Reference Standard Material :

Material	Serial No.	Certificate No.	Due date
1. Absorbance Standard set	32587	100509	28 Mar 2024
2. Absorbance Standard set	32590	100508	28 Mar 2024
3. Absorbance Standard set	8331	105939	28 Sep 2024
4. Wavelength Standard set	29829	94776	02 Sep 2023
5. Wavelength Standard set	29829	94777	02 Sep 2023

2. This certificate is valid only to the item calibrated on date and place of calibration.
3. This certificate is traceable to the International System of Unit maintained at :
   - National Physical Laboratory (NPL), The United Kingdom of Great Britain and Northern Ireland
   - National Institute of Standards and Technology (NIST), The United States of America
4. Spectral BandWidth : 5 nm
   Scan Speed : - nm/min

Calibration Results : without adjustment

Wavelength Accuracy

Certified Values of Reference Material (nm)	UUC Reading (nm)	Uncertainty of Measurement (± nm)	Coverage Factor *k*
361.40	361	0.59	2.00
447.20	446	0.59	2.00
537.00	536	0.59	2.00
638.00	637	0.59	2.00
740.51	741	0.59	2.00
807.04	807	0.59	2.00

[redacted]

Calibration Results : without adjustment

Photometric Accuracy

Wavelength (nm)	Certified Values of Reference Material (Abs)	UUC Reading (Abs)	Uncertainty of Measurement (±Abs)	Coverage Factor *k*
350.0	Zero	0.000	0.0046	2.00
	0.4246	0.423	0.0061	2.00
	Zero	0.000	0.0050	2.00
	0.6385	0.633	0.0055	2.00
440.0	Zero	0.000	0.0028	2.00
	0.5607	0.560	0.0030	2.00
	0.7336	0.733	0.0030	2.00
	1.0636	1.063	0.0030	2.00
546.1	Zero	0.000	0.0028	2.00
	0.5224	0.522	0.0028	2.00
	0.6856	0.684	0.0029	2.00
	0.9937	0.992	0.0028	2.00
635.0	Zero	0.000	0.0028	2.00
	0.5397	0.538	0.0028	2.00
	0.6832	0.680	0.0028	2.00
	0.9886	0.985	0.0028	2.00

Remark

- Each individual filter is measured against the empty filter holder (blank) used to zero the spectrophotometer
- The Potassium Dichromate filled cells are measured against a Perchloric acid blank.

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k* , providing a level of confidence of approximately 95 %.

-o0o-

[redacted]

TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000-29 FAX. 0-2719-9484

NSC-TISI-TIS17025
CALIBRATION 0008

Cert. No.: 23TM1173

Certificate of Calibration

Equipment :	Water Bath
Manufacturer :	Memmert
Model :	WB 22
Serial No. :	I505.0053
ID No. :	WAB-01
Submitted by :	Environment & Laboratory Co.,Ltd. 40 Soi Liangmueangnonthaburi 13, Talad Kwan, Mueang, Nonthaburi 11000
Location :	Room No. 303
Received Order :	12 July 2023
Calibration Date :	12 - 13 July 2023
Ambient Temperature :	(26 ± 10) °C
Relative Humidity :	(50 ± 30) %

[redacted]

Issue Date : 24 July 2023

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

Equipment : Water Bath
Condition As-Received : Used Item
Reference : 2307-0094OC-3

Cert. No.: 23TM1173

Procedure Used :-

Calibration were conducted using in-house calibration procedure CP-OT04 according to direct measurement method with Data Acquisition which connected with Industrial Platinum Resistance Thermometer (IPRT).

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-


Instrument	Serial No.	Cert. No.	Traceable	Due Date
1) Data Acquisition	MY44073381	23LM95	TPA	19 May 2024

2. This certificate is valid only to the item calibrated on date and place of calibration.
3. This certification is traceable to the International System of Unit.

Remark : TPA : Technology Promotion Association (Thailand - Japan)

Result of Calibration :- (*) Without Adjustment
Function of UUC* : Temperature Source
Heat transfer medium used : Water

	Environmental		AC Voltage Supply
	(°C)	(%R.H.)	(Volt)
Beginning of Calibration	30	47	220
Finished of Calibration	31	50	221

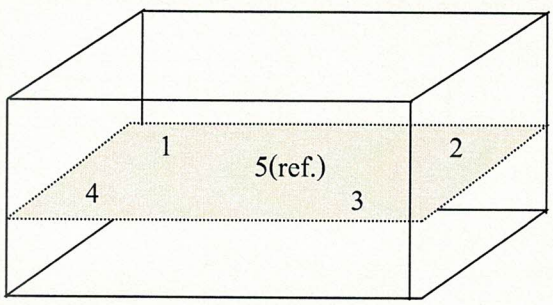

Front

Position :	Ref. Std. S/N.:
1	4803988-006
2	4803988-007
3	4804539-014
4	4804539-015
5(ref.)	4804539-016

[redacted]

a 1172193

Equipment : Water Bath
Condition As-Received : Used Item
Reference : 2307-0094OC-3
Result of Calibration :- (*) Without Adjustment
Function of UUC* : Temperature Source

Cert. No.: 23TM1173

Calibration point (°C)	UUC* Setting (°C)	UUC* Reading (°C)	Average* Standard Reading (°C) Position					Uncertainty (± °C)
			1	2	3	4	5 (ref.)	
44.5	44.5	44.5	44.507	44.503	44.498	44.509	44.502	0.15
60.0	60.0	60.0	59.914	59.928	59.912	59.899	59.894	0.15

Calibration point (°C)	Uniformity (°C)	Stability (± °C)	Coverage Factor *k*
44.5	0.039	0.023	2
60.0	0.098	0.042	2

Average* : The average of 30 values in each position.
Uniformity : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.
Stability : One-half of the greatest maximum difference of measured temperature at any one probe.
UUC* : Unit Under Calibration
Note : The reported uncertainty of measurement was included stability and excluded uniformity.

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor ***k***, providing a level of confidence of approximately 95 %.

-o0o-

[redacted]

a 1172192

TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL.0-2717-3000-29 FAX.0-2719-9484

NSC-TISI-TIS17025
CALIBRATION 0008

Certificate of Calibration

Cert.No.: 24CG774

Equipment :	Burette
Capacity :	50 mL
Serial No. :	-
ID. No. :	BUR-005
Manufacturer :	Witeg
Made in :	Germany
Submitted by :	Environment & Laboratory Co.,Ltd. 40 Soi Liangmueangnonthaburi 13 Talad Kwan, Mueang, Nonthaburi 11000
Ambient Temperature :	(20 ± 2.5) °C
Relative Humidity :	(50 ± 10) %
Barometric Pressure :	760 mmHg
Calibration Procedure :	ASTM E 542 - 01

[redacted]

Issue Date : 20 February 2024

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

Equipment : Burette
Received Date : 16 February 2024
Condition As-Received : Used Item
Calibration Date : 20 February 2024
Reference : 2402-0505DC-6

Cert.No.: 24CG774

Condition of this result of calibration

1. Reference Standard Instruments :

Instruments	Model	Serial No.	ID. No.	Certificate No.	Traceability	Due date
1) Balance	XP205DR	1126143764	140RC004	23MM538	TPA	15 Sep 2024
2) Thermo-Hygrograph	THDX-CE	00016540	140EC001	23H1275	TPA	09 June 2024
3) Thermometer	-	0834181	140EC005	23I948	TPA	10 Aug 2024

   This certification is traceable to SI Unit
2. The certificate is valid only to the item calibrated on date and place of calibration.
3. True value is converted to true volume at the standard temperature of 20 $^{\circ}$C

Calibration result :

Nominal capacity (mL)	Reading (mL)	Uncertainty (± mL)	*k* Factor
50	49.9765	0.010	2.00

Remark mL = cm^3

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k* , providing a level of confidence of approximately 95 %.

-o0o-