

เอกสารแนบ

9

เอกสารสอบเทียบเครื่องมือ



บริษัท ไมน์ เอ็นจิเนียริ่ง คอนซัลแตนท์ จำกัด
MINE ENGINEERING CONSULTANT CO.,LTD.

Analyzer Performance Test

Instrument of Status

Name	CO, SO ₂ , NO ₂ Analyzer	Brand	Thermo Environmental
No.	CO No. 1/ SO ₂ No. 1/ NO ₂ No. 1	Model	48 C / 43 C / 42 C
Date of Calibration	19 July 2024	Serial No.	CO-57041-31112
Dilutor Name	Dasibi Model 5008		SO ₂ -0335003718
Generator Air	API MODEL 701		NO ₂ -032620000000883

Standard Gas Details

Component	Concentration (ppm)	Cylinder No.	Expired Date
Carbon Monoxide (CO)	4535.0	EB0129027	29-Oct-27
Nitric Oxide (NO)	55.5	EB0129027	29-Oct-27
Sulfur Dioxide (SO ₂)	55.1	EB0129027	29-Oct-27

Calibration Status

Before Calibrate Result

Component	Unit	Reference Gas		Gas Analyzer Reading		Difference				Criteria
		Zero	Span	Zero	Span	Zero		Span		
						Value	%	Value	%	
CO	ppm	0.00	45.00	0.20	44.00	-0.20	-0.44	1.00	2.22	±5.0%of STD
NOx	ppm	0.00	400.00	0.09	396.70	0.00	0.00	3.30	0.83	±2.5%of STD
NO	ppm	0.00	400.00	0.10	397.40	-0.10	-0.03	2.60	0.65	±2.5%of STD
SO ₂	ppm	0.00	400.00	0.10	397.90	-0.10	-0.03	2.10	0.53	±2.5%of STD

After Calibrate Result

Component	Unit	Reference Gas		Gas Analyzer Reading		Difference				Criteria
		Zero	Span	Zero	Span	Zero		Span		
						Value	%	Value	%	
CO	ppm	0.00	45.00	0.00	45.00	0.00	0.00	0.00	0.00	±5.0%of STD
NOx	ppm	0.00	400.00	0.10	400.00	-0.10	-0.03	0.00	0.00	±2.5%of STD
NO	ppm	0.00	400.00	0.10	400.00	-0.10	-0.03	0.00	0.00	±2.5%of STD
SO ₂	ppm	0.00	400.00	0.00	400.00	0.00	0.00	0.00	0.00	±2.5%of STD

Calibrated by

Date

19/07/67



Approved by

Date

19/07/67



บริษัท ไมน์ เอ็นจิเนียริ่ง คอนซัลแตนท์ จำกัด
MINE ENGINEERING CONSULTANT CO.,LTD.

Analyzer Performance Test

Instrument of Status

Name	CO, SO ₂ , NO ₂ Analyzer	Brand	Thermo Environmental
No.	CO No. 2/ SO ₂ No. 2/ NO ₂ No. 2	Model	48 C / 43 C / 42 C
Date of Calibration	19 July 2024	Serial No.	CO-0531813056
Dilutor Name	Dasibi Model 5008		SO ₂ -0335003707
Generator Air	API MODEL 701		NO ₂ -03262000000886

Standard Gas Details

Component	Concentration (ppm)	Cylinder No.	Expired Date
Carbon Monoxide (CO)	4535.0	EB0129027	29-Oct-27
Nitric Oxide (NO)	55.5	EB0129027	29-Oct-27
Sulfur Dioxide (SO ₂)	55.1	EB0129027	29-Oct-27

Calibration Status

Before Calibrate Result

Component	Unit	Reference Gas		Gas Analyzer Reading		Difference				Criteria
		Zero	Span	Zero	Span	Zero		Span		
						Value	%	Value	%	
CO	ppm	0.00	45.00	0.20	44.10	-0.20	-0.44	0.90	2.00	±5.0%of STD
NOx	ppm	0.00	400.00	0.00	396.50	0.00	0.00	3.50	0.88	±2.5%of STD
NO	ppm	0.00	400.00	0.10	397.50	-0.10	-0.03	2.50	0.63	±2.5%of STD
SO ₂	ppm	0.00	400.00	0.10	398.10	-0.10	-0.03	1.90	0.47	±2.5%of STD

After Calibrate Result

Component	Unit	Reference Gas		Gas Analyzer Reading		Difference				Criteria
		Zero	Span	Zero	Span	Zero		Span		
						Value	%	Value	%	
CO	ppm	0.00	45.00	0.00	45.00	0.00	0.00	0.00	0.00	±5.0%of STD
Nox	ppm	0.00	400.00	0.00	400.00	0.00	0.00	0.00	0.00	±2.5%of STD
NO	ppm	0.00	400.00	0.10	400.00	-0.10	-0.03	0.00	0.00	±2.5%of STD
SO ₂	ppm	0.00	400.00	0.00	400.00	0.00	0.00	0.00	0.00	±2.5%of STD

Calibrated by

Date

19/07/67



Approved by

Date

19/07/67



SCARLET | TECH



Calibration Laboratory
3519

Certificate of Calibrator

for ST-120 Sound Calibrator

No. 20240708J669

Name of Product Sound Calibrator

Type ST-120

Serial Number ST120C0669E

Specification Class 1

Date 2024/07/16

Tested by



1. Outside: OK

2. Sound Pressure Level: 93.99 dB ; 114.05 dB

3. Frequency: 999.66 Hz

4. Distortion: 1.1 % ; 1.2 %

Environment conditions :

Air temperature : 25 °C

Relative humidity : 60 %

Static pressure : 101.8 kPa

Scarlet Tech Co., Ltd.



CERTIFICATE OF CALIBRATION

NO. 20240708148

Name of Product: Sound Level Meter
Model: ST-21D
Serial Number: 820797
Specification: Class 2
Conclusion: Pass
Date of calibration: 2024-07-17
Due Date: 2025-07-16



Calibrated by: [Redacted]

- I. This report certifies that all calibration equipment used in the test is traceable with the internal ISO 9001 procedures and meets all specification given in the Manual(s) or respectively surpass them, and applies only to the unit identified above.
II. This certificate is produced with advanced equipment & procedures which permit comprehensive quality assurance verification of all data supplied herein.
III. This certificate of calibration shall not be reproduced except in full, without written permission of the Scarlet Tech Co Ltd Taiwan.

1. Preliminary inspection: OK

2. Type & serial No. of Microphone: AWA14421A-000416

3. Adjustments to indicated sound levels:

Type of Calibrator: B&K 4231

Sound Pressure Level: 94.0 dB

4. Measuring up limit: 138 dBA

5. Frequency weightings (Acoustic signal tests for Z weighting, other electric signal tests.)

Equivalent Free-field Sound Level (reference environment conditions) 93.8 dB

Nominal frequency /Hz	Frequency weighting / dB			Nominal frequency /Hz	Frequency weighting / dB		
	A	C	Z		A	C	Z
20	-50.3	-6.3	-0.2	1000	0.0	0.0	0.0
31.5	-39.4	-2.9	0.0	2000	1.3	-0.1	0.0
63	-26.1	-0.8	0.0	4000	1.3	-0.6	0.1
125	-16.2	-0.2	0.0	8000	-1.2	-3.2	0.0
250	-8.6	0.0	0.0	12500	-11.0	-13.0	0.1
500	-3.2	0.0	0.0	/	/	/	/

6. Self-generated noise

Microphone replaced by electrical input signal device

24.5 dB(A)	25.6 dB(C)	33.5 dB(Z)
------------	------------	------------

7. F&S Weighting

Rate of the F weighting decrease (dB/s)	34.4
Rate of the S weighting decrease (dB/s)	4.3
Deviation of F&S	-0.1

8. Level Linearity (A-weighting at frequency 1 kHz)

Reference sound level 90.0 dB

Max error at 10dB steps upper reference sound level 0.1 dB

Max error at 1dB steps within 5dB of the upper limit linear operating range 0.0 dB

Max error at 10dB steps below reference sound level 0.1 dB

Max error at 1dB steps within 5dB upper the lower limit linear operating range 0.1 dB

9. Tone burst response (A Weighting) :

Single Toneburst duration /ms	Toneburst response /dB			
	LAFmax-LA	LASmax-LA	LAE-LA	LAeqT-LA
500	0.0	-4.0	-2.9	-7.0
200	-1.0	-5.9	-6.9	-7.0
2	-8.2	-26.9	-26.9	-7.0
0.25	-27.1	/	-36.1	-7.0

10. Peak C sound level (>500Hz) :

Cycle	One cycle	nominal value	Positive half	nominal value	Negative half	nominal value
LCpeak-LC(dB)	3.5	3.5	2.3	2.4	2.3	2.4

11. Overload indication: Pass

12. Statistical analysis function

Sweep signal maximum indicated sound level: 123.0 dB

Sweep amplitude: 40 dB

Scan cycle time: 60 S; Measurement period: 180 S

Items	Measured value/dB	Theoretical calculated value/dB	Error/dB
L _{Aeq,T}	113.3	113.4	-0.1
L ₅	121.0	121.0	0.0
L ₁₀	119.0	119.0	0.0
L ₅₀	103.0	103.0	0.0
L ₉₀	87.1	87.0	0.1
L ₉₅	85.1	85.0	0.1

Uncertainty of measurement results: 0.4 dB (k=2)

Environment conditions

:

Air temperature: 20 °C

Relative humidity: 50 %

Static pressure: 101.8 kPa

Test specifications:

1. All **Scartel's** Sound level Meter has been calibrated in accordance with the requirements as specified in ISO 17025 and the lab calibration procedure SMTP004-CA-152.
2. The electrical tests were performed using an electrical signal substituted for the microphone which was removed and replaced by an equivalent capacitance within a tolerance of ±20%.
3. The acoustic calibration was performed using an B&K 4226 sound calibrator and corrections was applied for the difference between the free-field and pressure responses of the Sound Level Meter.

References:

IEC 61672-3 Sound Level Meters Part 3: Periodic tests

ใช้เพื่อประกอบเล่มรายงาน โครงการวิจัยการพักอาศัยแปลง D1 (อาคาร D2)
โครงการฟื้นฟูเมืองชุมชนดินแดง ระยะที่ 3
ฉบับประจำเดือนมกราคม - มิถุนายน 2568



CERTIFICATE OF CALIBRATION

NO. 20240708149

Name of Product:	Sound Level Meter
Model:	ST-21D
Serial Number:	820798
Specification:	Class 2
Conclusion:	Pass
Date of calibration:	2024-07-17
Due Date:	2025-07-16

Calibrated by: [REDACTED]



- I. This report certifies that all calibration equipment used in the test is traceable with the internal ISO9001 procedures and meets all specification given in the Manual(s) or respectively surpass them, and applies only to the unit identified above.
- II. This certificate is produced with advanced equipment & procedures which permit comprehensive quality assurance verification of all data supplied herein.
- III. This certificate of calibration shall not be reproduced except in full, without written permission of the Scarlet Tech Co Ltd Taiwan.

1. Preliminary inspection: OK

2. Type & serial No. of Microphone: AWA14421A-000682

3. Adjustments to indicated sound levels:

Type of Calibrator: B&K 4231

Sound Pressure Level: 94.0 dB

Equivalent Free-field Sound Level (reference environment conditions) 93.8 dB

4. Measuring up limit: 138 dBA

5. Frequency weightings (Acoustic signal tests for Z weighting, other electric signal tests.)

Nominal frequency / Hz	Frequency weighting / dB			Nominal frequency / Hz	Frequency weighting / dB		
	A	C	Z		A	C	Z
20	-50.4	-6.1	-0.2	1000	0.0	0.0	0.0
31.5	-39.4	-3.1	0.0	2000	1.4	-0.1	0.0
63	-26.2	-0.8	0.0	4000	1.3	-0.6	0.0
125	-16.2	-0.2	0.0	8000	-1.2	-3.1	0.1
250	-8.6	0.0	0.0	12500	-11.0	-13.0	0.0
500	-3.2	0.0	0.0	/	/	/	/

6. Self-generated noise

Microphone replaced by electrical input signal device

24.6 dB(A)	26.4 dB(C)	37.0 dB(Z)
------------	------------	------------

7. F&S Weighting

Rate of the F weighting decrease (dB/s)	34.5
Rate of the S weighting decrease (dB/s)	4.2
Deviation of F&S	-0.1

8. Level Linearity (A-weighting at frequency 1 kHz)

Reference sound level 90.0 dB

Max error at 10dB steps upper reference sound level 0.1 dB

Max error at 1dB steps within 5dB of the upper limit linear operating range 0.0 dB

Max error at 10dB steps below reference sound level 0.1 dB

Max error at 1dB steps within 5dB upper the lower limit linear operating range 0.1 dB

9. Tone burst response (A Weighting) :

Single Toneburst duration /ms	Toneburst response /dB			
	LAFmax-LA	LASmax-LA	LAE-LA	LAeqT-LA
500	0.0	-4.0	-2.9	-7.0
200	-1.0	-7.4	-6.9	-7.0
2	-8.2	-26.9	-26.9	-7.0
0.25	-27.1	/	-36.1	-7.0

10. Peak C sound level (500Hz) :

One cycle	One cycle	nominal value	Positive half	nominal value	Negative half	nominal value
LCpeak-LC(dB)	3.5	3.5	2.3	2.4	2.3	2.4

11. Overload indication: Pass

12. Statistical analysis function

Sweep signal maximum indicated sound level: 123.0 dB

Sweep amplitude: 40 dB

Scan cycle time: 60 S; Measurement period: 180 S

Items	Measured value/dB	Theoretical calculated value/dB	Error/dB
L _{Aeq,T}	113.3	113.4	-0.1
L ₅	121.0	121.0	0.0
L ₁₀	119.0	119.0	0.0
L ₅₀	103.0	103.0	0.0
L ₉₀	87.1	87.0	0.1
L ₉₅	85.1	85.0	0.1

Uncertainty of measurement results: 0.4 dB (k=2)

Environment conditions

:

Air temperature: 20 °C

Relative humidity: 50 %

Static pressure: 101.8 kPa

Test specifications:

1. All **Scartlet's** Sound level Meter has been calibrated in accordance with the requirements as specified in ISO 17025 and the lab calibration procedure SMTP004-CA-152.
2. The electrical tests were performed using an electrical signal substituted for the microphone which was removed and replaced by an equivalent capacitance within a tolerance of ±20%.
3. The acoustic calibration was performed using an ASK 4226 sound calibrator and corrections was applied for the difference between the free-field and pressure responses of the Sound Level Meter.

References:

IEC 61672-3 Sound Level Meters Part 3: Periodic tests

ใช้เพื่อประกอบเล่มรายงาน โดยกรมการไฟฟ้าต๋ยแปลง D1 (อาคาร D2)
โครงการฟื้นฟูเมืองชุมชนดินแดง ระยะที่ 3
ฉบับประจำเดือนมกราคม - มิถุนายน 2568

CERTIFICATE OF CALIBRATION

Certificate No. : COF-047-67

Page 1 of 2 Pages

MEASUREMENT ITEM : Top Load Orifice
MANUFACTURER : TISCH
MODEL/TYPE : TE-5025A
SERIAL NUMBER : 2262
ID NUMBER : -
CONDITION AS-RECEIVED : Used item
CUSTOMER : Mine Engineering Consultant Co., Ltd.

Calibration procedure:

The Orifice gas flow device was calibrated against Standard Rotary Displacement Meter (Roots Meter) Model G65/IMC/W2-dp. The WI-CL-004 was used as a calibration guideline.

Traceability:

This certificate provides a traceability of the measurement to recognized the national standards and to realization of the international system of units (SI) through the NIMT (National Metrology Institute of Thailand) via Certificate number: MW-0063-23.

Uncertainty of Measurement:

The reported uncertainty of measurement is based on the standard uncertainty multiplied by a coverage factor $k=2$, Which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty has been determined in accordance with the GUM 'Evaluation of measurement data - Guide to the expression of uncertainty in measurement'

RECEIVED DATE : 27 Nov 2024
MEASUREMENT DATE : 28 Nov 2024
ISSUE DATE : 29 Nov 2024

ENVIRONMENTAL CONDITIONS:

Ambient condition in the laboratory are as follow:

Temperature : 23.0 ± 3.0 °C
Relative Humidity : 55.0 ± 15.0 %RH
Atmospheric Pressure : 1010 ± 10 hPa

CALIBRATION CONDITION:

Preconditioning : 24 hours at ambient conditions
Measurement Condition : The average values during measurement are 24.7 °C and 55.8 %RH.

NOTED: The certificate is valid only to the item calibrated on date and place of calibration.

TABULATION OF RESULTS:

The table on next page give the measured values.

Calibrated by:



Approved signatory:

Calibration Department Manager

MEASUREMENT RESULTS:

The Orifice gas flow device was calibrated by direct comparison method with the Standard Rotary Displacement Meter (Roots Meter). The Humid air was used as a medium in the system. The standard conditions are 25°C (298.15 K) and 760 mmHg for standard temperature and standard pressure, respectively.

Table 1: The results of Q Standard calibration data

Plate	Flow rate m^3/min	Pressure [Pa] mmHg	Temperature [Ta] °C	Temperature [Tm] °C	Δp_{meter} mmHg	$\Delta p_{Orifice}$ inH ₂ O	γ	Standard Flow [Q_s] m^3/min
1	0.702	759.268	24.51	23.58	55.802	1.742	1.320	0.653
2	1.001	759.347	24.52	23.63	61.117	3.511	1.875	0.924
3	1.117	759.363	24.59	23.82	43.208	4.628	2.152	1.056
4	1.164	759.452	24.69	23.96	31.142	5.207	2.282	1.120
5	1.410	759.442	24.78	24.11	30.680	7.686	2.772	1.356

Slope (m): 2.06451
Intercept (b): -0.02907
Correlation coefficient (r): 0.99986
Uncertainty ($k=2$): 0.015 m^3/min

Table 2: The results of Q actual calibration data

Plate	Flow rate m^3/min	Pressure [Pa] mmHg	Temperature [Ta] °C	Temperature [Tm] °C	Δp_{meter} mmHg	$\Delta p_{Orifice}$ inH ₂ O	γ	Standard Flow [Q_a] m^3/min
1	0.702	759.268	24.51	23.58	55.802	1.742	0.826	0.652
2	1.001	759.347	24.52	23.63	61.117	3.511	1.173	0.923
3	1.117	759.363	24.59	23.82	43.208	4.628	1.347	1.056
4	1.164	759.452	24.69	23.96	31.142	5.207	1.429	1.119
5	1.410	759.442	24.78	24.11	30.680	7.686	1.736	1.356

Slope (m): 1.29307
Intercept (b): -0.01819
Correlation coefficient (r): 0.99986
Uncertainty ($k = 2$): 0.015 m^3/min

End of Certificate of Calibration



Calibration Certificate

Part Number: 721A2601
Description: Micromate with DIN Geophone
Serial Number: UM22390
Calibration Date: SEP 29 2024
Calibration Reference Equipment: 714J7402

Instantel certifies that the above product was calibrated in accordance with the applicable Instantel procedures. These procedures are part of a quality system that is designed to assure that the product listed above meets or exceeds Instantel specifications.

Instantel further certifies that the measurement instruments used during the calibration of this product are traceable to the National Institute of Standards and Technology; or National Research Council of Canada. Evidence of traceability is on file at Instantel and is available upon request.

The environment in which this product was calibrated is maintained within the operating specifications of the instrument.

Please note that the sensor check function is intended to check that the sensors are connected to the unit, installed in the proper orientation and sufficiently level to operate properly. This function should not be confused with a formal calibration, which requires the sensors be checked against a reference that is traceable to a known standard.

Instantel recommends that products be returned to Instantel or an authorized service and calibration facility for annual calibration.


Calibrated By: _____



309 Legget Drive, Ottawa, Ontario, K2K 3A3, (613) 592-4642

ใช้เพื่อรับรองการสอบเทียบ
โดย Instantel
สำหรับผลิตภัณฑ์ D1 (อาคาร D2)
วันที่ 2563

Frequency Response of UM22390

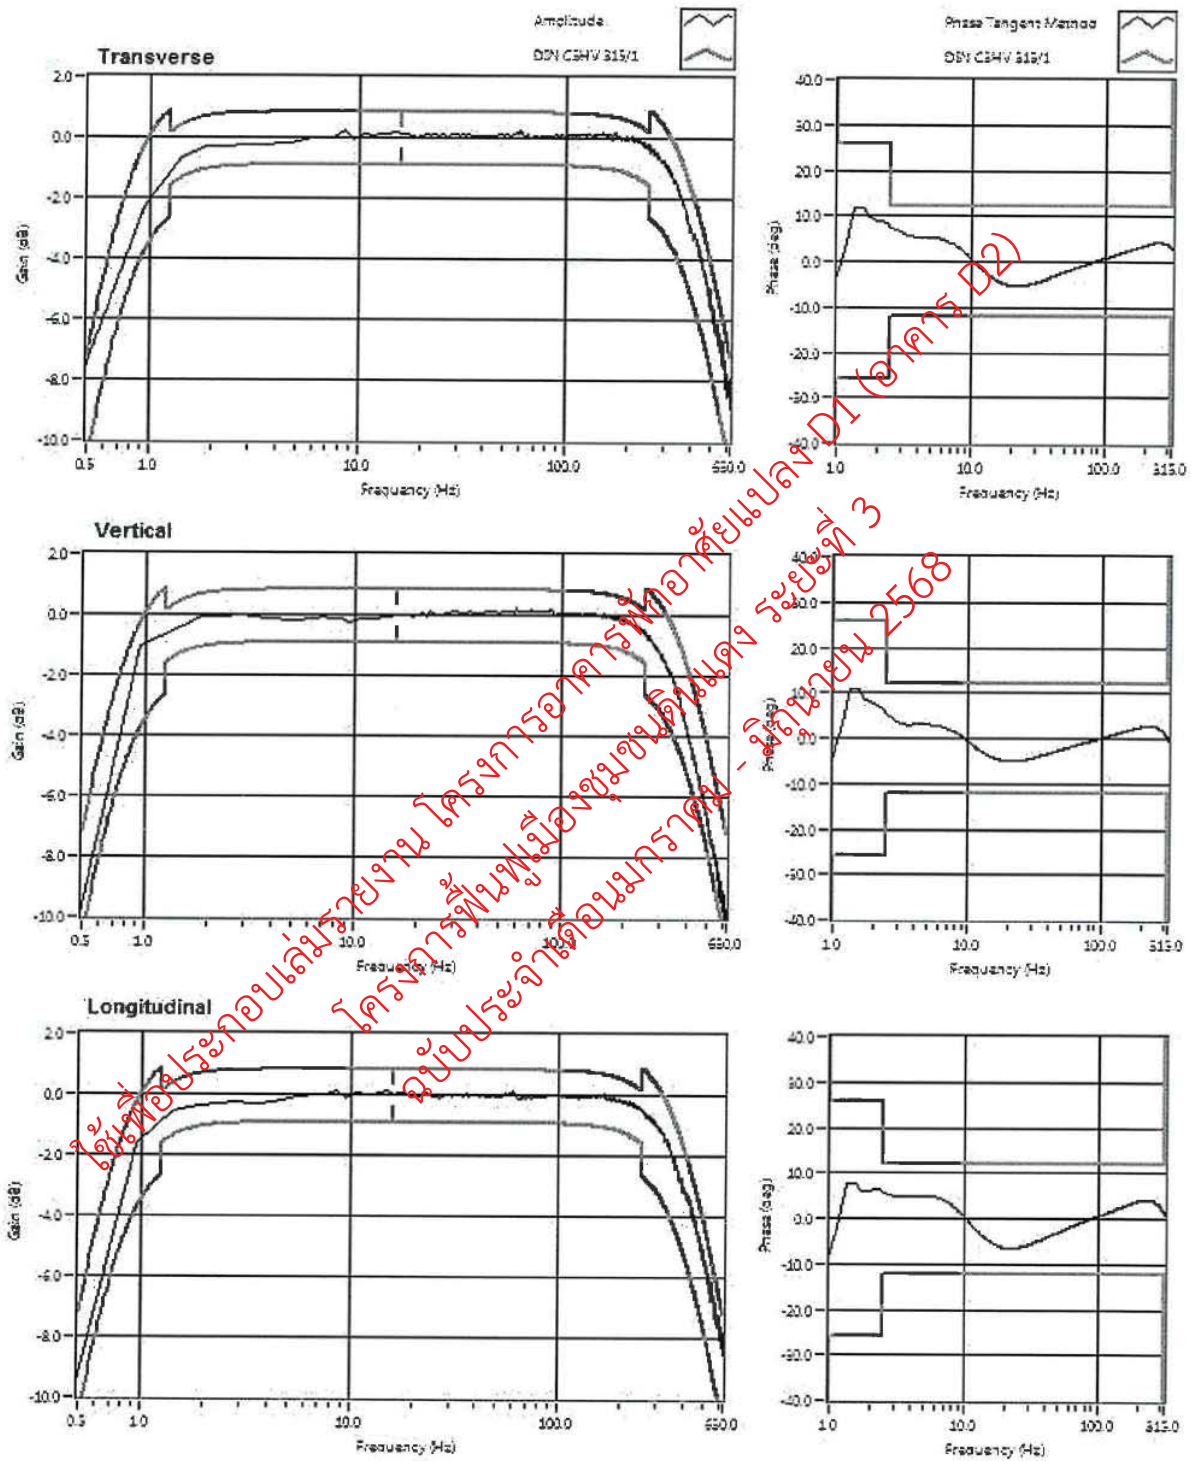

Calibration Certificate

Part Number: 721A2601
Description: Micromate with DIN Geophone
Serial Number: UM22389
Calibration Date: SEP 29 2024
Calibration Reference Equipment: 714J7402

Instantel certifies that the above product was calibrated in accordance with the applicable Instantel procedures. These procedures are part of a quality system that is designed to assure that the product listed above meets or exceeds Instantel specifications.

Instantel further certifies that the measurement instruments used during the calibration of this product are traceable to the National Institute of Standards and Technology; or National Research Council of Canada. Evidence of traceability is on file at Instantel and is available upon request.

The environment in which this product was calibrated is maintained within the operating specifications of the instrument.

Please note that the sensor check function is intended to check that the sensors are connected to the unit, installed in the proper orientation and sufficiently level to operate properly. This function should not be confused with a formal calibration, which requires the sensors be checked against a reference that is traceable to a known standard. Instantel recommends that products be returned to Instantel or an authorized service and calibration facility for annual calibration.


Calibrated By: _____



309 Legget Drive, Ottawa, Ontario, K2K 3A3, (613) 592-4642

ใช้เพื่อรับรองการสอบเทียบผลิตภัณฑ์ D1 (อาคาร D2)
วันที่ 2560

Frequency Response of UM22389

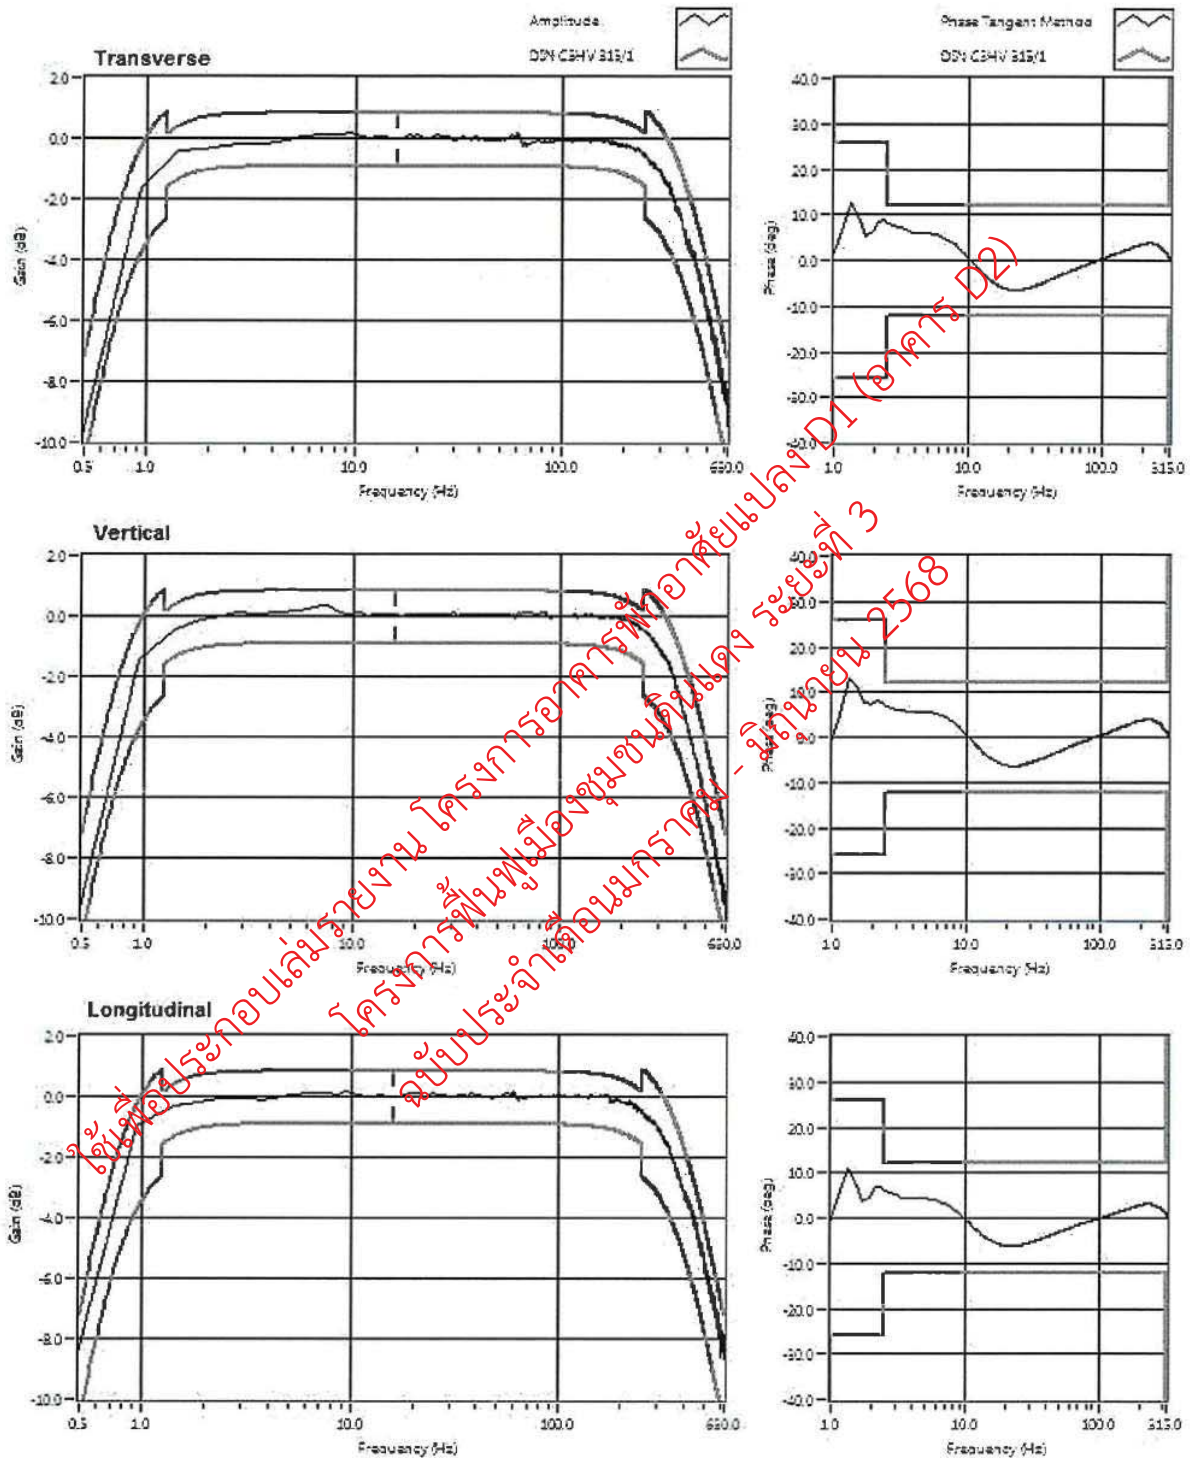



CALIBRATION LABORATORY Co., LTD.



CERTIFICATE OF CALIBRATION

FOR

NOMENCLATURE : ELECTRONIC BALANCE
MANUFACTURER : SARTORIUS
MODEL / TYPE : AZ214
SERIAL NO. : 28092281[MEC-LAB01]
CLID. NO. : 362101621
JOB CONTROL NO. : 240718075309
CALIBRATION SERVICE : ☐ IN-LABORATORY ☒ ON-SITE

CUSTOMER : MINE ENGINEERING CONSULTANT CO., LTD.

DATE OF RECEIVED : 18 July 2024

DATE OF ISSUED : 25 July 2024

The report of calibration shall not be reproduced except in full without approval of the Calibration Laboratory Co., Ltd.

Calibrated By : Nattawadee Baengpech
Calibration Engineer

Approved By :

Authorized Signatory
25 July 2024



This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to the International System of Units (SI)

Certificate No. Q24075309

F3-011-05/12-23

page 1 of 3



@clccalibration



CLC
Accredited
ISO/IEC 17025

CALIBRATION LABORATORY Co., LTD.



REPORT OF CALIBRATION

FOR

NOMENCLATURE : ELECTRONIC BALANCE
MANUFACTURER : SARTORIUS
MODEL / TYPE : AZ214
SERIAL NO. : 28092281[MEC-LAB01]
LOCATION SITE : LABORATORY
DATE OF CALIBRATION : 20 July 2024

ENVIRONMENT CONDITIONS :

Temperature : 23 °C to 24 °C

Relative Humidity : 53 % to 56 %

PROCEDURE USED :

This instrument was calibrated under procedure No. CLC-CPMB-01 based on EURAMET/cg-18/Version 4.0 (11/2015).

The calibration was performed by Comparison with Weight Set which maintained by the Calibration Laboratory Co., Ltd.

REFERENCE STANDARD USED :

1. Weight Set, Phoenix Class E2 S/N. WBS-SET-E2-01.
2. Weight, Sartorius Class E2 S/N. 44329129, 43529037, 44329167, 43529293.

TRACEABILITY :

1. The measurements are traceable to International System of Units (SI), through National Institute of Metrology (Thailand).

Certificate No. MM-0123-22, Due Date 22 August 2024.

2. The measurements are traceable to International System of Units (SI), through Sartorius Lab Instruments GmbH & Co. KG.

Certificate No. M141607, M141608, M141609, M141611. Due Date 15 September 2025.

UNCERTAINTY :

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor complies with the table which for a normal distribution corresponds to a coverage probability of approximately 95%. It has been evaluated according to the "Evaluation of the Uncertainty of Measurement in Calibration (EA-4/02 M:2022)"

Certificate No. Q24075309

F3-011-05/12-23

page 2 of 3



@clccalibration

CONDITION OF CALIBRATION ITEM : RECEIVED IN GOOD OPERATIONAL CONDITION

MEASUREMENT RESULTS : (X) without adjustment () adjustment

CALIBRATION DATA



1. Error of indications

Nominal Test Value (g)	Conventional mass (g)	Display Value (g)	Error of Balance (g)	Uncertainty \pm (mg)	Coverage factor k
Unload	0.0000	0.0000	0.0000	0.04	2,28
0.0010	0.0010	0.0010	0.0000	0.07	2,00
0.0100	0.0100	0.0100	0.0000	0.07	2,00
0.1000	0.1000	0.1000	0.0000	0.07	2,00
1.0000	1.0000	1.0000	0.0000	0.07	2,00
5.0000	5.0000	5.0000	0.0000	0.07	2,00
10.0000	10.0000	10.0001	+0.0001	0.07	2,00
50.0000	50.0000	50.0000	0.0000	0.11	2,00
100.0000	100.0000	100.0000	0.0000	0.18	2,00
150.0000	150.0000	150.0000	0.0000	0.26	2,00
200.0000	200.0001	200.0001	-0.0001	0.33	2,00

2. Repeatability of indications

Nominal Test Value (g)	Standard Deviation of Reading (g)
200.0000	0.00005

3. Effect of eccentric application of a load on the indication

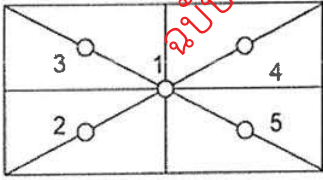 						
Nominal Test Value (g)	Display Value (g)					Maximum Difference of Center Value (g)
	Position 1	Position 2	Position 3	Position 4	Position 5	
50.0000	50.0000	50.0001	50.0001	50.0000	50.0000	0.0001

Note. The Scope of Accredited ANAB Certificate No. ACDM-2814 Version 012 Page 49 of 67

This report is valid for the above stated instrument/s only.

End of Certificate

Certificate No. Q24075309

F3-011-05/12-23

page 3 of 3





CALIBRATION LABORATORY Co., LTD.



CERTIFICATE OF CALIBRATION

FOR

NOMENCLATURE : OVEN
MANUFACTURER : MEMMERT
MODEL / TYPE : UF110
SERIAL NO. : B418.1125 [MEC-LAB05]
CLID. NO. : 332102410
JOB CONTROL NO. : 340718075311
CALIBRATION SERVICE : ☐ IN LABORATORY ☒ ON-SITE

CUSTOMER : MINE ENGINEERING CONSULTANT CO., LTD.

DATE OF RECEIVED : 18 July 2024

DATE OF ISSUED : 25 July 2024

The report of calibration shall not be reproduced except in full without approval of the Calibration Laboratory Co., Ltd.

Calibrated By :

Wenick Inchaisri

Calibration Engineer

Approved By :

Authorized Signatory

25 July 2024



This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to the International System of Units (SI)

Certificate No. Q24075311

F3-011-05/12-23

page 1 of 4



@clccalibration



REPORT OF CALIBRATION

FOR

NOMENCLATURE : OVEN
MANUFACTURER : MEMMERT
MODEL / TYPE : UF110
SERIAL NO. : B418.1125[MEC-LAB05]
LOCATION SITE : LABORATORY
DATE OF CALIBRATION : 20 July 2024

ENVIRONMENT CONDITIONS :

Temperature : 27 °C to 28 °C

Relative Humidity : 50% to 54 %

PROCEDURE USED :

This instrument was calibrated under procedure No. **CLC-CPT-07** based on **TLAS G-20** as calibration guidelines.

The calibration was performed by using Hydra Data Logger which maintained by the Calibration Laboratory Co., Ltd.

REFERENCE STANDARD USED :

Hydra Data Logger, Fluke Model 2635A, S/N. 5499551.

TRACEABILITY :

The measurements are traceable to International System of Units (SI) , through Calibration Laboratory Co., Ltd.

Certificate No. Q23116630, Due Date 25 October 2024.

UNCERTAINTY :

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor complies with the table which for a normal distribution corresponds to a coverage probability of approximately 95 %.

It has been evaluated according to the "Evaluation of the Uncertainty of Measurement in Calibration (EA-4/02 M:2022)"

Certificate No. Q24075311

F3-011-05/12-23



CONDITION OF CALIBRATION ITEM : RECEIVED IN GOOD OPERATIONAL CONDITION

MEASUREMENT RESULTS : (X) without adjustment () adjustment

The table in the following gives the calibration results and associated measurement uncertainties of the measuring oven.

CALIBRATION DATA

1. OVEN PERFORMANCE

DUC		Measured Uniformity	Measured Stability	Measured Overall
Setting (°C)	Indicating (°C)	(°C)	(°C)	Variation (°C)
85.0	85.0	0.63	0.44	1.47
104.0	104.0	0.78	0.11	1.10
180.0	180.0	1.63	0.13	2.30

ใช้เพื่อประกอบเล่มรายงาน โครงการอาคารพักอาศัยแปลง D1 (อาคาร D2)
 โครงการฟื้นฟูเมืองชุมชนดินแดง ระยะที่ 3
 ฉบับประจำเดือนมกราคม - มิถุนายน 2568


CALIBRATION DATA

2. TEMPERATURE DISTRIBUTION

DUC		Measured Temperature (°C)@Probe No.9 is Ref.									Uncertainty \pm (°C)	Coverage factor k
Setting (°C)	Indicating (°C)	1	2	3	4	5	6	7	8	9		
85.0	85.0	84.49	85.15	84.90	85.11	84.84	84.95	84.67	84.81	85.06	0.57	2,00
104.0	104.0	103.32	104.25	103.90	104.17	103.80	103.96	103.57	103.88	104.07	0.46	2,00
180.0	180.0	178.91	181.05	180.19	180.81	179.78	180.41	179.68	180.05	180.48	0.57	2,00

Technical Note : W = 56 cm, D = 40 cm, H = 48 cm.

Note. The Scope of Accredited ANAB Certificate No. ACDM-2814 Version 012 Page 58 of 67

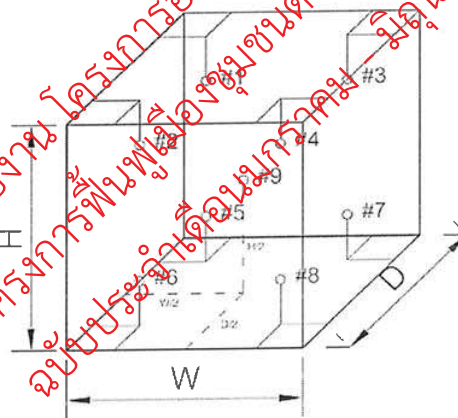

This report is valid for the above stated instrument/s only.

End of Certificate

Certificate No. Q24075311

F3-011-05/12-23

page 4 of 4





CLC
Accredited
ISO/IEC 17025

CALIBRATION LABORATORY Co., LTD.



CERTIFICATE OF CALIBRATION

FOR

NOMENCLATURE : pH METER
MANUFACTURER : EUTECH INSTRUMENTS
MODEL / TYPE : PH700
SERIAL NO. : 983068/93X218814/93X052911 [MEC-LAB06]
CLID. NO. : 372200480
JOB CONTROL NO. : 240748075312
CALIBRATION SERVICE : ☐ IN-LABORATORY ☒ ON-SITE

CUSTOMER : MINE ENGINEERING CONSULTANT CO., LTD.

DATE OF RECEIVED : 18 July 2024

DATE OF ISSUED : 25 July 2024

The report of calibration shall not be reproduced except in full without approval of the Calibration Laboratory Co., Ltd.

Calibrated By :

Sukkasem Sechanart

Wenick Inchaisri

Calibration Engineer



Approved By :

Authorized Signatory

25 July 2024

This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to the International System of Units (SI)

Certificate No. Q24075312

F3-011-05/12-23

page 1 of 4



@clccalibration



REPORT OF CALIBRATION

FOR

NOMENCLATURE : pH METER
MANUFACTURER : EUTECH INSTRUMENTS
MODEL / TYPE : PH700
SERIAL NO. : 98306893X21881493X052911[MEC-LAB06]
LOCATION SITE : LABORATORY
DATE OF CALIBRATION : 20 July 2024

ENVIRONMENT CONDITIONS :

Temperature : 21°C to 22°C

Relative Humidity : 50% to 53%

PROCEDURE USED :

This instrument was calibrated under procedure No. CLC-CPTH-01, CLC-CPTH-03 based on ASTM E 644-04 as calibration guidelines. The calibration was performed by direct measurement with Certified Reference Material (CRM) and comparison with Micro Calibration Bath, Precision Thermometer and IPRT which maintained by the Calibration Laboratory Co., Ltd.

REFERENCE STANDARD USED :

1. pH Standard Solution, NIMT TRM CODE TRM-S-2002, TRM CODE TRM-S-2003, TRM CODE TRM-S-2007.
2. pH Standard Solution, Control Company Catalog Number 06664260, 11754256, Lot Number CC787362.
3. Micro Calibration Bath, Kambic Model OBM-LT S/N. 18015718.
4. IPRT, SDL Model T100-450-1D S/N. K0897A-1-19.
5. Precision Thermometer, Wika Model CTH 7000 S/N. 014471/18.





CALIBRATION LABORATORY Co., LTD.



TRACEABILITY :

1. The measurements are traceable to International System of Units (SI) , through National Institute of Metrology (Thailand).
Lot Number. 260124, 040822 , 120124. Due Date 04 March 2025.
2. The measurements are traceable to International System of Units (SI) , through Control Company
Certificate No. 4281-14495731 , Due Date 27 September 2025.
3. The measurements are traceable to International System of Units (SI) , through Calibration Laboratory Co., Ltd.
Certificate No. Q23136343 , Due Date 25 December 2024.
4. The measurements are traceable to International System of Units (SI) , through National Institute of Metrology (Thailand).
Certificate No. TT-0100-23, Due Date 23 August 2024.
5. The measurements are traceable to International System of Units (SI) , through Thailand Institute of Scientific and Technological Research (TISTR). Certificate No. PSL-T 0961866, Due Date 30 August 2024.

UNCERTAINTY :

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor complies with the table which for a normal distribution corresponds to a coverage probability of approximately 95 %.

It has been evaluated according to the "Evaluation of the Uncertainty of Measurement in Calibration (EA-4/02 M:2022)"





CLC
Accredited
ISO/IEC 17025

CALIBRATION LABORATORY Co., LTD.



CONDITION OF CALIBRATION ITEM : RECEIVED IN GOOD OPERATIONAL CONDITION

MEASUREMENT RESULTS : (X) without adjustment () adjustment

The table in the following gives the calibration results and associated measurement uncertainties of pH meter.

CALIBRATION DATA

1. pH METER RESULT @ 25 °C

Standard pH Buffer Solution (pH)	pH Meter Reading (pH)	pH Meter Reading (mV)	Correction (pH)	Uncertainty of pH Measurement (± pH)	k Factor
1.684	1.67	306	+0.014	0.013	2,20
4.003	4.00	173.0	+0.003	0.013	2,15
7.005	7.02	-4.7	-0.015	0.015	2.06
10.015	9.98	-176.3	+0.035	0.016	2,05

Note. The Scope of Accredited ANAB Certificate No. ACDM-2814 Version 012 Page 4 of 67

2. TEMPERATURE RESULT [THERMISTOR]

Immersion depth (mm)	Actual Temperature (°C)	°C Reading (°C)	Correction (°C)	Uncertainty ± (°C)
100	25.00	25.00	0.00	0.13

Note. Probe Ø 4 mm

Materials : Metal Sheath.

The Scope of Accredited ANAB Certificate No. ACDM-2814 Version 012 Page 56 of 67

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor of $k = 2,00$.

This report is valid for the above stated instrument/s only.

End of Certificate

Certificate No. Q24075312

F3-011-05/12-23

page 4 of 4



@clccalibration

Certificate No. T/O 680070

Date of issue : 21-Mar-2025

Equipment Description : Incubator
Equipment Model : i250-DS
Equipment Serial No. : 0408-0315-0025
I.D. No. or Control No. : -
Manufacturer : Entech Industrial Solution Co.,Ltd.
Customer Name : MINE ENGINEERING CONSULTANT CO.,LTD.
Customer Address :

Total pages of certificate : 2 pages
Instrument Receiving Date : 21-Mar-2025
Receiving No. : O-250091
Environmental Conditions : All of the measurement were carried out in the working area
Temperature : (25 ± 15) °C
Humidity : (55 ± 30) % RH
Voltage : (220 ± 22) VAC

Calibration Place :

Calibration Procedure No. : This instrument was calibrated by comparison of indication with the Standard Resistance thermometer according to calibration TLAS G20, work instruction no WI-CL-18-C

The calibration certificate expended uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k, which for a normal distribution corresponds to a coverage probability of approximately 95%

The standard uncertainty of measurement has been determined in accordance with M 3003

The expression uncertainty and confidence in measurement

This certificate is applied only to item under test environmental condition.

This calibration certificate may not be reproduced other than in full except with the permission of the issuing laboratory. Calibration certificates without signature and seal are not valid and The results relate only to the items tested/calibrated.

This calibration certificate documents are traceability to national standards, which realize the unit of measurement according to the International system of units (SI).

Date of Calibration : 21-Mar-2025

Calibration Engineer

Technical Manager

Certificate No. : T/O 680070


The Reference Standard Instrument :-

Instrument	Model	Serial No.	Cert No.	Due date
1) Data logger with RTD Probe	Agilent 34972A	MY41187730 MY60008352	PSL-T 0409-1/68 PSL-T 0409-3/68	23-Feb-2026 23-Feb-2026

Measured room conditions

Temperature :	Minimum: 20.5 °C	Maximum: 22.4 °C
Humidity :	Minimum: 50.8 %RH	Maximum: 65.5 %RH
Voltage :	Minimum: 219.9 VAC	Maximum: 223.1 VAC
Fresh Air Setting:	off	

Sensor Position :

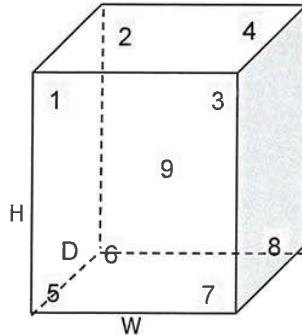

Working Space of chamber :

(Inside Dimensions) W x D x H : 490 mm x 480 mm x 1190 mm

Sensor Installation Details :

- Sensor Number 1 to 8 installed approximately 50 mm From each wall.
- Sensor Number 9 installed approximately geometric of the chamber.

Results : The measurement results of the calibration were reported in the table below.

(*) Without adjustment

() After adjustment

UUC* Setting	UUC* Reading	Temperature Reading of Standard Sensor Sensor Position								
(°C)	(°C)	1	2	3	4	5	6	7	8	9
20.0	20.0	20.11	20.15	19.90	20.05	19.97	20.03	19.76	19.76	20.00


UUC* Setting	UUC* Reading	Temperature Uniformity	Temperature Stability	Overall Variation	Uncertainty of Measurement	Coverage Factor
(°C)	(°C)	(°C)	(± °C)	(°C)	(± °C)	K
20.0	20.0	0.49	0.33	0.90	0.56	2.02

UUC* = Unit Under Calibration

Remark :-

- Temperature reading of Standard Sensors shown in the table were taken from the average of Standard reading at each position.
- Temperature Uniformity was calculated from the difference between the maximum and minimum of actual temperature reading from all reference sensors at the same time.
- Temperature Stability was calculated from the maximum stability of nine positions, and formula of Stability is $[(\text{Maximum Temperature Value} - \text{Minimum Temperature Value}) / 2]$
- Overall Variation was calculated from the difference between the maximum and minimum measured temperature throughout observation time.

End of Report



BUCHI Certificate Final Test Inspection

Unit : BÜCHI BÜCHI Kjelflex K-360

Serial number 1000281014

Examination Procedure

- 1. Visual control of the glass parts and the unit**
 - No scratches on the coated surface or splinters on the glass parts
 - Mounted in accordance to the specific drawing
- 2. Security tests**
 - High voltage test in accordance with EN 61010-1:2002 (IEC 61010-1:2001) (VDE 0411)
 - Ground connection test in accordance with EN 61010-1:2002 (IEC 61010-1:2001) (VDE 0411)
 - Safety door sensor checked
- 3. Functional tests**
 - Electronics**
 - Electronic modul is tested with the checking device PG157
 - Connector plugs are working
 - Operating panel**
 - Display is working
 - All buttons of the keypad are working
 - Pump testing**
 - All pumps are working
 - All pumps (exception: water pump of the steam generator) are precalibrated
 - Valve testing**
 - All valves are working
 - Steam generator testing**
 - The steam generator is filled with water
 - The steam generator valve is working
 - The amount of distillate corresponds to specifications
 - Further testing**
 - Beeper is working
- 4. Unit configuration and completeness of order checked**

BÜCHI Labortechnik AG hereby declares that this unit is in accordance with the specifications

Signature, Date:

Packing List

Unit : K-360 Plastik Basic



151111113001000281014111

Serial Number

1000281014

Page 1(1)

Item	Pieces	Description	
043410	3.0000	Canister 10L thin-walled Kanister 10L dünnwandig	OK
043603	1.0000	Packing parts K-360 Beipackteile K-360	OK
047871	1.0000	Suppl. sheet distillation unit Beiblatt Distillation Unit	OK
010020	1.0000	Power cable type USA, 3 pole 120V Anschlusskabel USA W 120V	OK
11592548	1.0000	Kjeldahl Practice Guide en Kjeldahl Practice Guide en	OK
093176	1.0000	Operation Manual K-360 english Bedienungsanleitung K-360 englisch	OK

Packed by

ใช้เพื่อประกอบเล่มรายงาน โครงการอาหารฟ้าอาศัยแปลง D1 (อาคาร D2)
โครงการฟื้นฟูเมืองชุมชนดินแดง ระยะที่ 3
ใช้ประจำเดือนมกราคม - มิถุนายน 2568



BUCHI Certificate
Final Test Inspection

Unit : BÜCHI Scrubber K-415

Serial number 1000281005

Examination Procedure

- 1. Visual control of the glass parts and the unit**
 - No scratches or splinters on the glass parts
 - Mounted in accordance to the specific drawing

OK
- 2. Security tests**
 - High voltage test in accordance with EN 61010-1 (IEC 1010)
 - Ground connection test in accordance with EN 61010-1 (IEC 1010)

OK
- 3. Functional tests**
 - Bypass valve open: Pressure is 0 - 65 mbar below the atmospheric pressure
 - Bypass valve closed: Pressure is 400 mbar (+/- 10 %) below the atmospheric pressure

OK
- 4. Completeness of order checked**

OK

BUCHI Labortechnik AG hereby declares that this unit is in accordance with the specifications

Signature, Date:

BU
TE
CO

Packing List

Unit : K-415 TripleScrub 230V



151111112781000281005111

Serial Number

1000281005

Page 1(1)

Item	Pieces	Description	
11057332	1.0000	Tray for adsorption storage Ablage für Adsorption	OK
048355	1.0000	Silicone hose D6/9 L=3m Silikonschlauch D6/9 L=3,0m	OK
033701	1.0000	Glass wool 30g Glaswolle 30g	OK
028737	2.0000	Hose clamp Anschlussklemme	OK
11064971	1.0000	Activated Charcoal 2-6mm, 150g Aktivkohle 2-6mm, 150g	OK
010020	1.0000	Power cable type USA, 3 pole 120V Anschlusskabel USA W 120V	OK
11593505	1.0000	Operation Manual K-415 english Bedienungsanleitung K-415 english	OK

Packed by

ใช้เพื่อประกอบเล่มรายงาน โครงการอาคารพักอาศัยแปลง D1 (อาคาร D2)
โครงการฟื้นฟูเมืองชุมชนดินแดง ระยะที่ 3
ฉบับประจำเดือนมกราคม - มิถุนายน 2568



BUCHI Certificate
Final Test Inspection

Unit : BÜCHI Kjeldigester K-446

Serial number 1000281006

Examination Procedure

- 1. Visual control of the glass parts and the unit**
 - No scratches on the coated surface
 - Mounted in accordance to the specific drawing

OK
- 2. Security tests**
 - High voltage test in accordance with EN 61010-1 (IEC 1010)
 - Ground connection test in accordance with EN 61010-1 (IEC 1010)

OK
- 3. Functional tests**

Operating panel

 - All buttons are working
 - Cooling system is working after the instrument has been switched on

OK

Connector plugs

 - Scrubber connector is working

OK

Heating element

 - Heating-up temperature 420 °C is reached after 40 minutes
 - Temperature calibration at 420 °C (3 measuring points)

OK
- 4. Completeness of order checked**

BÜCHI Labortechnik AG hereby declares that this unit is in accordance with the specifications

Signature, Date:

Packing List

Unit : K-446 Kjeldigester standard



151111112791000281006111

Serial Number

1000281006

Page 1(1)

Item	Pieces	Description	
11059833	1.0000	Packing parts Kjeldigester K-446/K-449 Beipackteile K-446/K-449	OK
037377	5.0000	Sample tubes 300 ml (set of 4) Probengläser 300 ml (Set à 4 Stück)	OK
11059754	1.0000	Rack 20 cpl. Rack 20 kpl.	OK
11058955	1.0000	Aspiration device Kjeldigester K-446/K-449 Absaugereinheit K-446/K-449	OK
040444	1.0000	Weighing boat 20pcs. Wägeschiffchen 20 Stk.	OK
010020	1.0000	Power cable type USA, 3 pole 120V Anschlusskabel USA W 120V	OK
11058825	1.0000	Fume collection tube with ball joint Dampfsammelrohr mit Kugelschiff	OK
11592548	1.0000	Kjeldahl Practice Guide en Kjeldahl Practice Guide en	OK
11593546	1.0000	Operation Manual K-446/K-449 english Bedienungsanleitung K-446/K-449 englisch	OK
11593549	1.0000	Supplementary sheet Kjeldigester K-446/K-449 Beiblatt K-446/K-449	OK

Packed by

ใช้เพื่อประกอบเล่มรายงาน โครงการอาคารพักอาศัยแบบ D1 (อาคาร D2)
โครงการฟื้นฟูเมืองชุมชนดินแดง ระยะที่ 3
ฉบับประจำเดือนมกราคม - มิถุนายน 2568



Certificate of Calibration

Equipment: SPECTROPHOTOMETER
Model: SP-2100
Serial No. (or ID.): KJ0G05083001 (MET-SP 01/46)
Manufacturer: HACH
Condition: In Condition

Certificate No.: C06240454
Issued Date: 16 October 2024
Job No.: WO-00045898
Page: 1 of 2

Customer: M E T CO.,LTD.

Environment Condition:

Temperature	26.1	°C	±	0.2	°C
Humidity	67.3	%RH	±	2.1	%RH

Calibration Place: M E T CO.,LTD. (Laboratory Room)

Calibration By: Mr. Nattapat Rungruang

Calibration Date: 16 October 2024

The Method used: In house method, CAL-WI-24, base on ASTM E 275-08 and ASTM E 387-04

Traceability: This certificate is traceable to the CRM maintained by National Institute of Standards and Technology (NIST) through Starna Scientific Limited.

The standard for Wavelength Certificate No. 113620 and 113619

The standard for Photometric Certificate No. 113650

Person in charge

Authorized signatory

This certificate is issued the units of measurement according to the International System of Units (SI). It provides traceability of measurement to international or national standard or other recognized national standard laboratories.

The measurement uncertainty stated is the expanded uncertainty which is obtained from the standard uncertainty multiplied by the coverage factor ($k=2$) to provide a level of confidence of approximately 95%. It is determined in accordance with the Guide to Expression of Uncertainty in Measurement (GUM).

These results may be affected by deviations from specified conditions. The results relate only to the items tested, calibrated or sampled. The report shall not be reproduced except in full without approval of DKSH Technology Limited.

บริษัท ดีเคเอสเอช เทคโนโลยี จำกัด
DKSH Technology Limited

Calibration Results:
Without Adjustment

Wavelength Accuracy (nm), The spectral bandwidth of Std at 4 nm and UUC at 4 nm

Standard Wavelength	Unit Under Calibration	Correction	Uncertainty
334.22	335	-0.78	0.59
418.48	419	-0.52	0.59
536.90	536	0.90	0.59
637.94	637	0.94	0.59
748.28	748	0.28	0.59
879.70	879	0.70	0.59

Photometric Accuracy (Absorbance)

Wavelength	Standard absorbance	Unit Under Calibration	Correction	Uncertainty
420 nm	0.0000	0.0007	-0.0070	0.0045
	0.5797	0.5789	0.0007	0.0045
	0.7119	0.714	-0.0021	0.0045
	1.0124	1.015	-0.0026	0.0045
440 nm	0.0000	0.001	-0.0010	0.0045
	0.5634	0.564	-0.0006	0.0045
	0.7001	0.704	-0.0039	0.0045
	0.9955	1.002	-0.0065	0.0045
465 nm	0.0000	0.000	0.0000	0.0045
	0.5239	0.523	0.0009	0.0045
	0.6613	0.660	0.0013	0.0045
	0.9395	0.941	-0.0015	0.0045
546.1 nm	0.0000	0.000	0.0000	0.0045
	0.5212	0.518	0.0032	0.0045
	0.6977	0.692	0.0057	0.0045
	0.9927	0.985	0.0077	0.0045
590 nm	0.0000	0.000	0.0000	0.0045
	0.5548	0.552	0.0028	0.0045
	0.7732	0.767	0.0062	0.0045
	1.1021	1.093	0.0091	0.0045
635 nm	0.0000	0.000	0.0000	0.0045
	0.5621	0.560	0.0021	0.0045
	0.7629	0.758	0.0049	0.0045
	1.0873	1.081	0.0063	0.0045

บริษัท ดีเคเอสเอช เทคโนโลยี จำกัด
DKSH Technology Limited

The End of Certificate

ใบตรวจสอบสภาพเครื่องวัดสิ่งแวดล้อม

เลขที่ใบงาน: WO-00045898

ชนิดเครื่องมือ: SPECTROPHOTOMETER

รุ่น: SP-2100

หมายเลขเครื่อง: KJ0G05083001

ตรวจสอบ (รับ)		รายการตรวจเช็ค	ตรวจสอบ (ส่ง)		หมายเหตุ
16 Oct 2024			16 Oct 2024		
ปกติ	ไม่ปกติ		ปกติ	ไม่ปกติ	
		<i>General</i>			
<input checked="" type="checkbox"/>	<input type="checkbox"/>	1. ความสมบูรณ์เครื่อง	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	2. ความสะอาด (ช่องใส่ตัวอย่าง, ภายใน-นอกเครื่อง)	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	3. สวิตช์ ปิด - เปิด เครื่อง (On-Off Swicth)	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	4. ปุ่มกด (Keypad)	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	5. หน้าจอ (Display, Screen Contrast)	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
		<i>Spectrophotometer</i>			
<input type="checkbox"/>	<input type="checkbox"/>	6. แรงดันไฟฟ้า (Battery Backup) ≥ 2.5 VDC	<input type="checkbox"/>	<input type="checkbox"/>	
<input type="checkbox"/>	<input type="checkbox"/>	7. ตัวหมุนเลือกความยาวคลื่น (Wavelength Control)	<input type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	8. ความยาวคลื่น (Wavelength Check)	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input type="checkbox"/>	<input type="checkbox"/>	9. แหล่งกำเนิดแสง (UV $< 3,000$ hour)	<input type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	10. แหล่งกำเนิดแสง (Visible $< 5,000$ hour)	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	11. ช่องวัดหลายตัวอย่าง (Carousel Module)	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
		<i>pH Meter and Conductivity Meter</i>			
<input type="checkbox"/>	<input type="checkbox"/>	12. อิเล็กโทรด (Electrode and Connection Cable)	<input type="checkbox"/>	<input type="checkbox"/>	
<input type="checkbox"/>	<input type="checkbox"/>	13. ระดับสารละลายใน Electrode (Level KCl)	<input type="checkbox"/>	<input type="checkbox"/>	
<input type="checkbox"/>	<input type="checkbox"/>	14. ฝาปิดกันผง Electrode (Dust Protection Hood)	<input type="checkbox"/>	<input type="checkbox"/>	
<input type="checkbox"/>	<input type="checkbox"/>	15. ขาจับอิเล็กโทรด (Stand)	<input type="checkbox"/>	<input type="checkbox"/>	
		<i>Turbidimeter</i>			
<input type="checkbox"/>	<input type="checkbox"/>	16. ค่าความขุ่นที่ต่ำสุด (No Sample)	<input type="checkbox"/>	<input type="checkbox"/>	
<input type="checkbox"/>	<input type="checkbox"/>	17. ระดับการส่องสว่างของแสง (≥ 2.5 ไม่เกิน 3.0)	<input type="checkbox"/>	<input type="checkbox"/>	
		<i>Automatic titrator</i>			
<input type="checkbox"/>	<input type="checkbox"/>	18. สภาพ Piston Burettes	<input type="checkbox"/>	<input type="checkbox"/>	
<input type="checkbox"/>	<input type="checkbox"/>	19. Function Rinsing and Dosing	<input type="checkbox"/>	<input type="checkbox"/>	
<input type="checkbox"/>	<input type="checkbox"/>	20. ระบบท่อสายยางและอุปกรณ์ประกอบ	<input type="checkbox"/>	<input type="checkbox"/>	

เพิ่มเติม/ขอแนะนำ :

Service Engineer

Introduction to Mérieux NutriSciences AQ

To all our Valued Customers,

Following Mérieux NutriSciences' [recent acquisition](#) of Bureau Veritas' Food Testing Activities*, we are writing to inform you of an important change regarding BVAQ Lab (Thailand) Ltd. Effective 25 March 2025, the legal entity will be renamed "**MNAQ Lab (Thailand) Ltd.**" Or เอ็มเอ็นเอควิ แล็บ (ประเทศไทย) จำกัด and will trade as Mérieux NutriSciences / Merieux NutriSciences AQ.

During this transition period, you may continue to receive invoices and reports bearing our current company name and logo. However, please be assured that this is a temporary measure, and we will be updating our branding on all documents once the ISO/IEC 17025 accreditation is updated.

All other details, such as our contact information, DBD business registration, and tax details, will be updated. To ensure a seamless transition, we kindly request your assistance in updating our supplier profile on your system to reflect our new company name. Please let us know if you require any specific documentation or information from us to facilitate this update.

We appreciate your continued partnership and look forward to working with you under our new company name. Should you have any questions or if there are any points you would like to discuss further at this time, please do not hesitate to contact your dedicated customer service representatives at

Kind regards,

General Manager (Thailand)

**As part of the global transaction, Mérieux NutriSciences will assume Bureau Veritas' role in the joint venture with AsureQuality operating in Southeast Asia, working as trusted partners helping the food industry to make food systems safer, healthier, and more sustainable. Further details of this joint venture, currently trading as BVAQ, will be communicated in the coming months.*

About Mérieux NutriSciences:

At Mérieux NutriSciences, we leverage over 50 years of scientific and entrepreneurial expertise to answer food industry needs. Today's global challenges transform the way food is produced, marketed and consumed, which is why we know our clients need more than reliable analytical results; they need practical and innovative solutions that will contribute to make food systems safer, healthier and more sustainable. Present worldwide, we are more than 100 accredited laboratories and a team of over 8,000 committed employees. We strongly believe that together, we can create solutions to offer our planet: BETTER FOOD. BETTER HEALTH. BETTER WORLD. For more information, visit

About AsureQuality:

AsureQuality offers the broadest range of food assurance services in New Zealand, supporting the food and primary production sectors reaching global markets. New Zealand Government owned, and with over 100 years' experience, AsureQuality has built a trusted reputation for delivering expert services and value for customers across the entire food supply chain. For more information, visit



CALIBRATION CERTIFICATE

Date of Issue Jun 28, 2024

Cert No. 24/2415

Site Calibration

Order No. 24060337

Customer Bureau Veritas AQ Lab (Thailand) Limited

Place of Calibration Incubation Room

Description Incubator

Model IN110

Serial No. D415.0797

ID.No. CHM000181

Date of Receipt Jun 24, 2024

Date of Calibration Jun 24, 2024

Environment

Temperature (Min) 22.8 °C (Max) 25.2 °C

Relative Humidity (Min) 44.7 %RH (Max) 58.5 %RH

Calibration Method

WI-17 : The reference thermometer was placed into the chamber and measurement was performed based on AS-2853.

The temperature scale in use at this laboratory is the International Temperature Scale of 1990.

Standard

1) Data Acquisition with Sensor Model 34972A S/N. MY49010059, Certificate No. QR24-0874, Calibrated by Quality Reborn Co., Ltd., ONAC Calibration No. 0292. Due Date Apr 24, 2025.

This certificate is traceable to SI unit.



CALIBRATION CERTIFICATE


Date of Issue Jun 28, 2024

Site Calibration

Cert No. 24/2415

Order No. 24060337

Results (without adjustment)

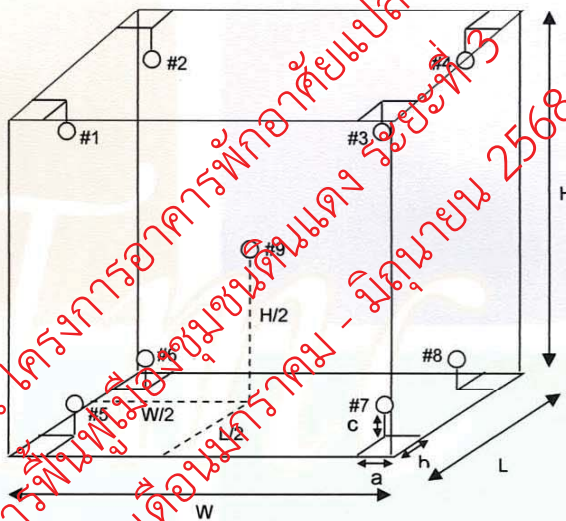

Position of reference thermometers were placed

Note

- 1). Dimension (W x L x H) is 56 x 40 x 48 cm.
- 2). Stability - greatest one half of difference between max peak and min peak of each reference probe measured temperature obtained during the calibration interval.
- 3). Uniformity - the maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady state conditions. The reference sensor should preferably be located at the geometric center of the chamber.



CALIBRATION CERTIFICATE

Date of Issue Jun 28, 2024

Cert No. 24/2415

Site Calibration

Order No. 24060337

Results (without adjustment)

Cal Point (°C)	UUC Setting (°C)	UUC Reading (°C)	Reference Thermometer (°C)	Stability \pm (°C)	Uniformity (°C)	Uncertainty \pm (°C)
35.0	35.0	35.0	Position 1	35.138	0.067	0.253
			Position 2	35.099		
			Position 3	35.075		
			Position 4	35.187		
			Position 5	35.173		
			Position 6	34.988		
			Position 7	34.878		
			Position 8	34.965		
			Position 9	34.970		

The stability and uniformity was taken into account in the measurement uncertainty stated.

The above results are valid exclusively for calibration samples as mentioned in the report.


The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor $k=2$, providing a level of confidence of approximately 95%. The uncertainty evaluation has been carried out in accordance with ONAC requirements.

APPROVED SIGNATORY :

[]

[]

[]

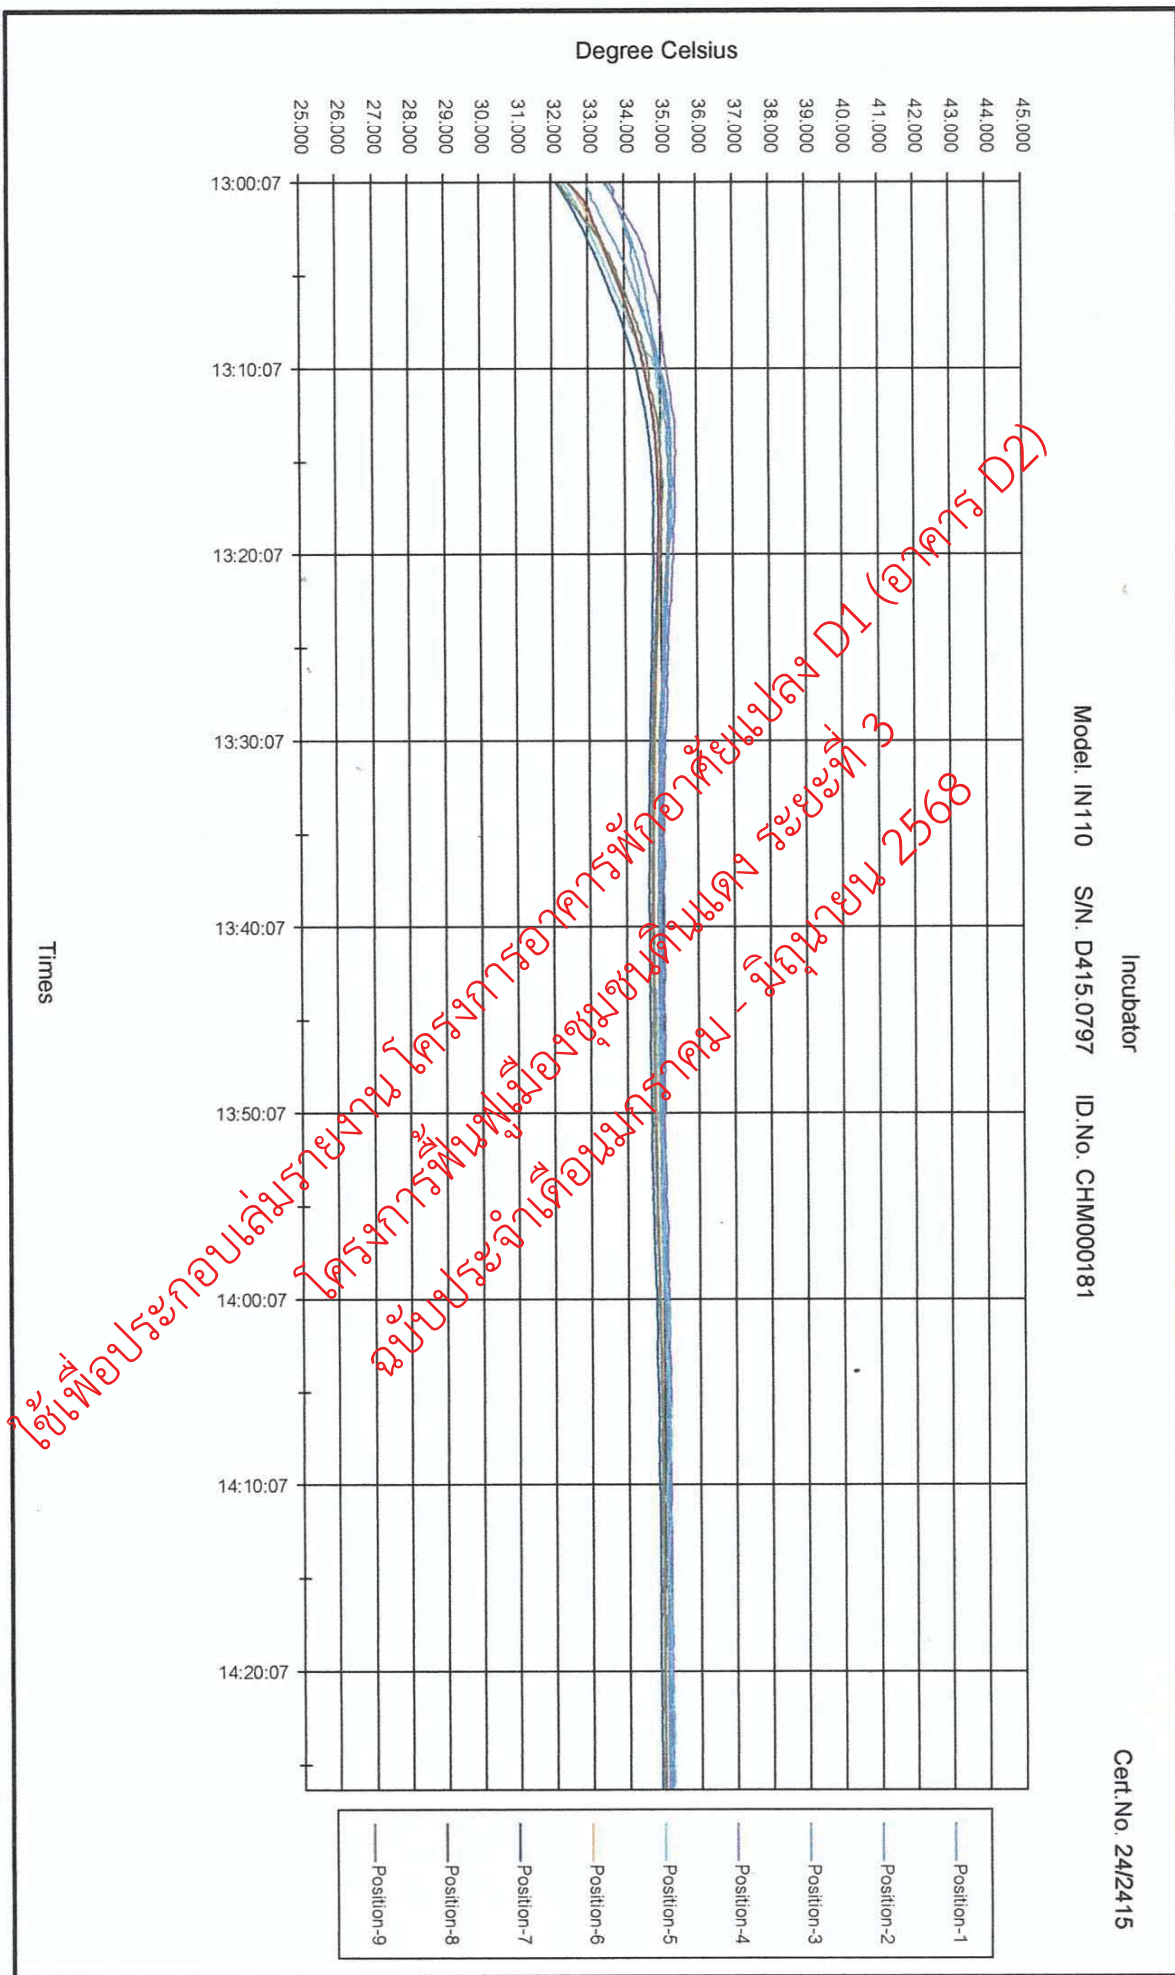



CALIBRATION CERTIFICATE

Date of Issue Jun 28, 2024

Cert No. 24/2418

Site Calibration

Order No. 24060337

Customer Bureau Veritas AQ Lab (Thailand) Limited

Place of Calibration Incubation Room

Description Water Bath

Model SC100

Serial No. 0152187501160414

ID.No. CHM000205

Date of Receipt Jun 24, 2024

Date of Calibration Jun 24, 2024

Environment

Temperature	(Min)	22.8	°C	(Max)	25.2	°C
Relative Humidity	(Min)	44.7	%RH	(Max)	58.5	%RH
Line Voltage	(Min)	227.2	VAC	(Max)	229.6	VAC

Calibration Method

WI-18 The reference thermometer was placed into the chamber and measurement was performed based on AS-2853.

The temperature scale in use at this laboratory is the International Temperature Scale of 1990.

Standard

1) Data Acquisition with Sensor Model 34972A S/N. MY49007789, Certificate No. QR24-0186, Calibrated by Quality Reborn Co., Ltd., ONAC Calibration No. 0292. Due Date Jan 23, 2025.

This certificate is traceable to SI unit.



CALIBRATION CERTIFICATE


Date of Issue Jun 28, 2024

Site Calibration

Cert No. 24/2418

Order No. 24060337

Results (without adjustment)

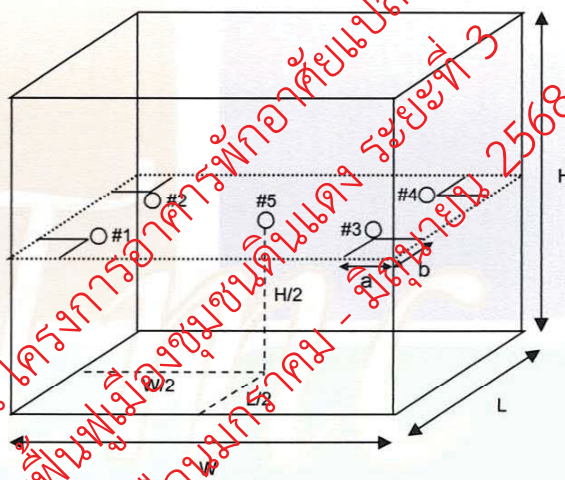

Position of reference thermometers were placed

Note.

1. Dimension (W x L x H) is 30 x 34 x 20 cm.
2. Stability - greatest one half of difference between max peak and min peak of each reference probe measured temperature obtained during the calibration interval.
3. Uniformity - the maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady state conditions. The reference sensor should preferably be located at the geometric center of the chamber.



CALIBRATION CERTIFICATE

Date of Issue Jun 28, 2024

Cert No. 24/2418

Site Calibration

Order No. 24060337

Results (without adjustment)

Cal Point (°C)	UUC Setting (°C)	UUC Reading (°C)	Reference Thermometer (°C)	Stability \pm (°C)	Uniformity (°C)	Uncertainty \pm (°C)
44.5	44.5	44.5	Position 1 44.490	0.020	0.043	0.13
			Position 2 44.494			
			Position 3 44.491			
			Position 4 44.499			
			Position 5 44.503			

The stability and uniformity was taken into account in the measurement uncertainty stated.

The above results are valid exclusively for calibration samples as mentioned in the report.

The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor $k=2$, providing a level of confidence of approximately 95%. The uncertainty evaluation has been carried out in accordance with ONAC requirements.


APPROVED SIGNATORY :

[]
[]
[]

Cert.No. 24/2418

Water Bath

Model. SC100 S/N. 0152187501160414 ID.No. CHM000205

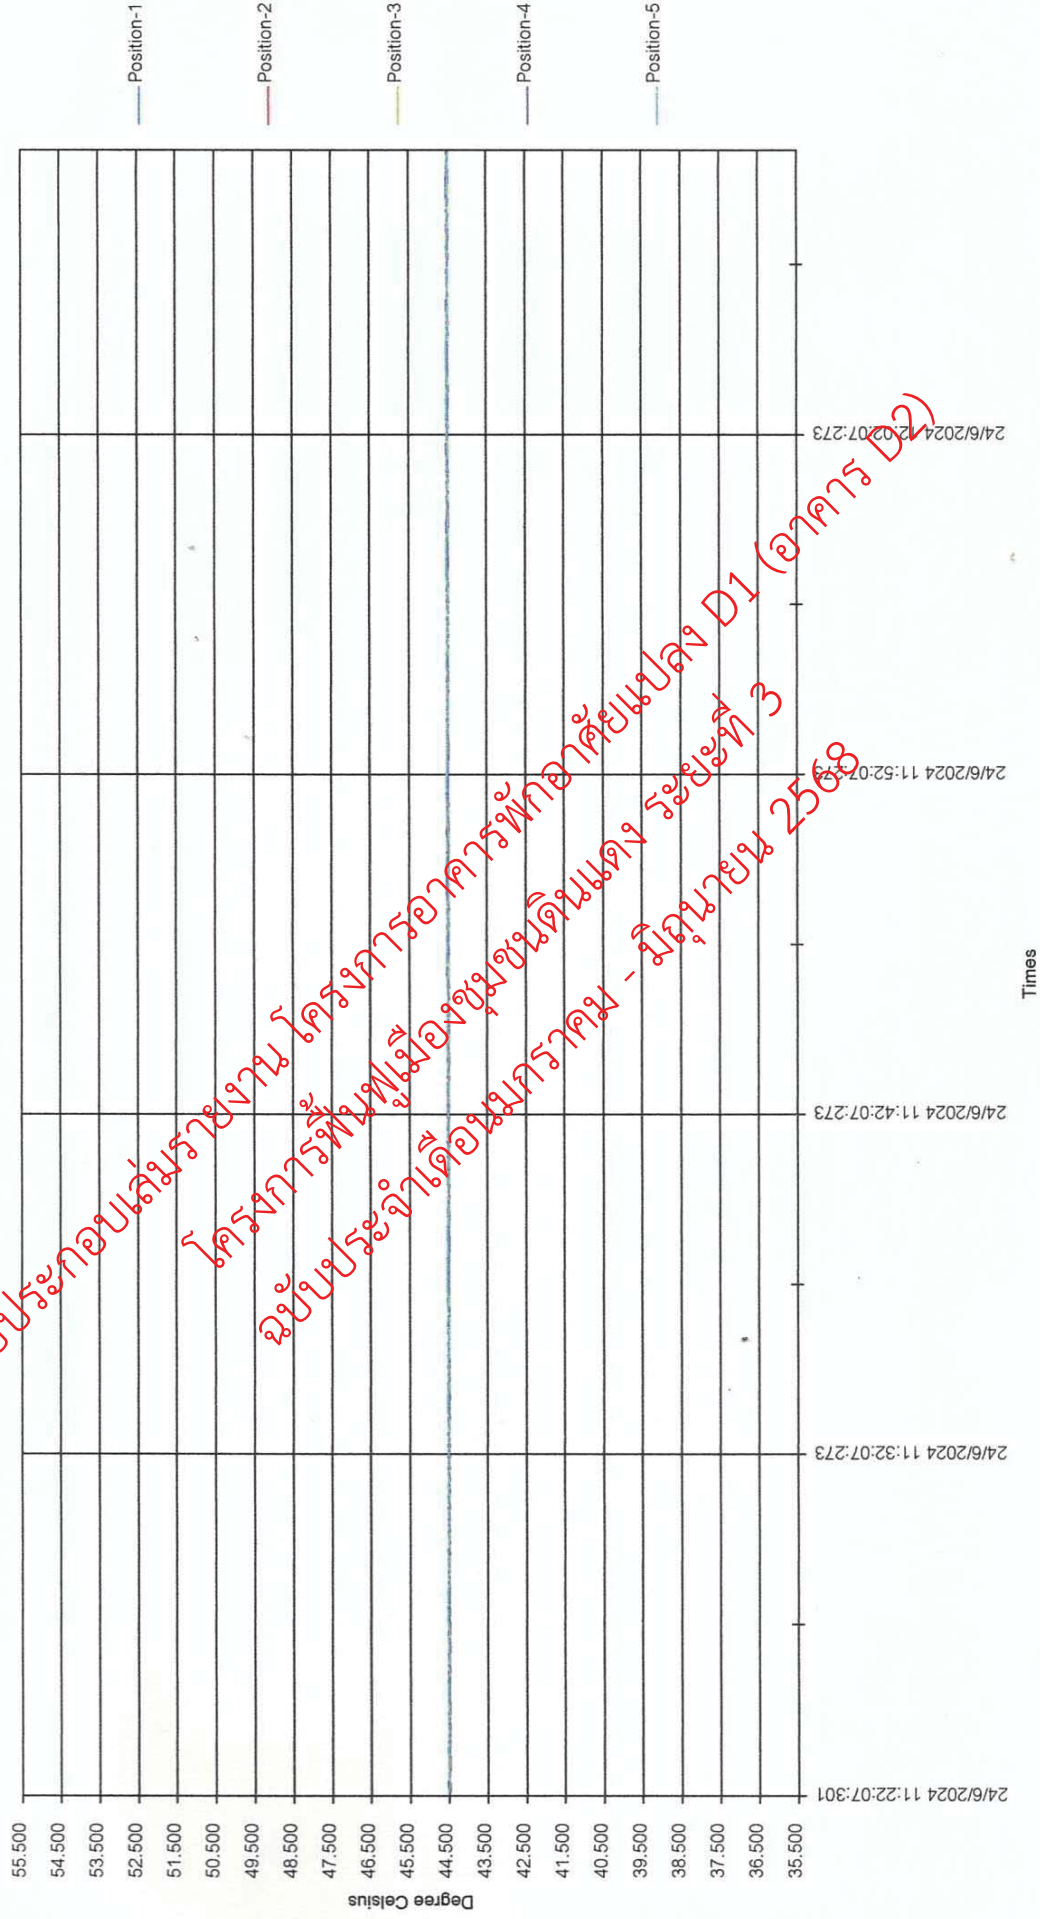



CERTIFICATE OF CALIBRATION

Issue Date : 29 February 2024
Certificate No. : 24-0256-007
Work Order No. : 24/0256

Customer Name : Bureau Veritas AQ Lab (Thailand) Limited

Date of Received : 28 February 2024

Date of Calibration : 28 February 2024

Instrument Details :
Description : Water Bath
Manufacturer : Julabo
Model : CORIO C
Serial No. : 10289054
ID No. : CHM000352
Resolution : 0.1 °C
Location : Laboratory

Calibration Method : This instrument was calibrated by insert standard thermometer into the liquid bath according to calibration procedure CWI-T-11 in-house methods based on ASTM E715-80 (Reapproved 2006)

Environmental Conditions :

Temperature : Area Monitoring between 15°C to 40°C

Humidity : Area Monitoring between 30%RH to 85%RH

Line Voltage : Area Monitoring 220 VAC \pm 10%

Traceability of Measurement :

This certificate of calibration documents the traceability to national standard, which realize the unit of measurement according to the International system of Units (SI) and The temperature scale in use at this laboratory is The International Temperature scale of 1990.

Calibrated by :

Calibration Engineer

Approved by :

Asst. Laboratory Manager

This certificate may not be reproduced other than in full except with the prior written approval of Crystal Calibration Sales and Service Co., Ltd.





CERTIFICATE OF CALIBRATION

Issue Date : 29 February 2024

Certificate No. : 24-0256-007

Work Order No. : 24/0256

Details of calibration

1. Reference Standards Instrument

Instrument	Model	Serial No. / ID No.	Certificate No.	Due Date
Data Acquisition unit	34972A	MY57006241	23-1150-002	02 September 2024
Sensor type	RTD	Channel 106 to 110	23-1150-002	02 September 2024

2. Certificate traceable

: This certificate traceable to The International System of Unit refer to
Crystal Calibration Sales and Service Co., Ltd. (NAC Calibration No. 0260)

3. Condition of item

: Used

4. Calibration site

: On-site

5. Result of Calibration

: Without Adjustment

6. Evaluate Condition

: Time Constant : 1 hour 33 Minute At Cal. point 44.5 °C

Type of Control : PID Control

Circulate pump value : Fixed Circulate


Testing liquid bath use media is Water

7. Calibration note

The results reported in this certificate refer to the condition of instrument on
the process into the steady state of Liquid Bath

8. Sensors Installation Diagram

:

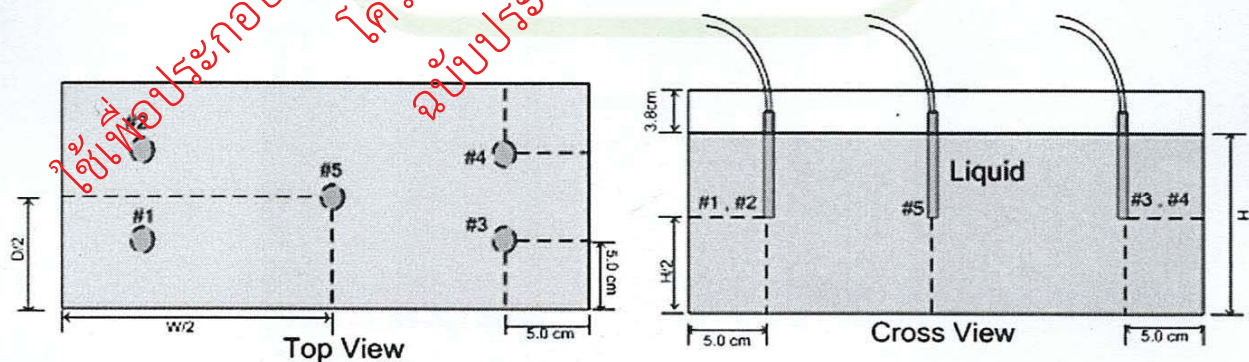

Position Diagrams



CERTIFICATE OF CALIBRATION

Issue Date : 29 February 2024

Certificate No. : 24-0256-007

Work Order No. : 24/0256

Result of Temperature Distribution and Performance Check

Table 1 : Reporting of Temperature

Calibration point (°C)	Average Measured Temperature (°C) @ Sensor No. (Sensor No.5 is REF)					Uncertainty ± (°C)
	#1	#2	#3	#4	#5	
44.5	44.46	44.46	44.45	44.45	44.48	0.13

Table 2 : Reporting of Characterization Result

Indicator Set point (°C)	Indicator Reading (°C)			Stability ± (°C)	Uniformity (°C)	Overall variation (°C)
	MAX	MIN	Average			
44.5	44.5	44.5	44.5	0.06	0.05	0.07

Note :

Calibrate items in good condition and this report customer request and accepted in certificate

The reference sensor is preferably located of the center of bath

The measured temperature data readout by software "Benchlink Datalogger 3"

The quoted uncertainty include " Stability " and exclude " Loading effect (20% of Temp Uniformity) "

Stability - one-half of the greatest maximum difference of measured temperatures at any one sensor.

Uniformity - the maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the bath under steady state conditions.

Overall Variation - The difference of the maximum and minimum measured temperatures throughout observation time.

Indicating Temperature - the average reading of indicating device that forms the integral part of the enclosure.

This result of calibration was found accurate as shown on date and place of calibration only.

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k=2$ providing a level of confidence of approximately 95%.



CERTIFICATE OF CALIBRATION

Issue Date : 29 February 2024

Certificate No. : 24-0256-007

Work Order No. : 24/0256

Result of Temperature Distribution and Performance Check

Table 1 : Reporting of Temperature

Calibration point (°C)	Average Measured Temperature (°C) @ Sensor No. (Sensor No.5 is REF)					Uncertainty ± (°C)
	#1	#2	#3	#4	#5	
44.5	44.46	44.46	44.45	44.45	44.48	0.13

Table 2 : Reporting of Characterization Result

Indicator Set point (°C)	Indicator Reading (°C)			Stability ± (°C)	Uniformity (°C)	Overall variation (°C)
	MAX	MIN	Average			
44.5	44.5	44.5	44.5	0.06	0.05	0.07

Note :

Calibrate items in good condition and this report customer request and accepted in certificate

The reference sensor is preferably located of the center of bath

The measured temperature data readout by software "Benchlink Datalogger 3"

The quoted uncertainty include " Stability " and exclude " Loading effect (20% of Temp Uniformity) "

Stability - one-half of the greatest maximum difference of measured temperatures at any one sensor.

Uniformity - the maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the bath under steady state conditions.

Overall Variation - The difference of the maximum and minimum measured temperatures throughout observation time

Indicating Temperature - the average reading of indicating device that forms the integral part of the enclosure.

This result of calibration was found accurate as shown on date and place of calibration only.

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k=2$ providing a level of confidence of approximately 95%.



Instrument Name: Incubator
Manufacturer: Hettich
Model: Hett Cube 400R
Serial No.: 0000166-03
ID No.: B-IN-19
Calibration Date: 2-Sep-24
Calibration by: AMARC
Certificate No.: 24-111504
จุดที่ใช้งาน: $36 \pm 1^\circ\text{C}$
เกณฑ์ยอมรับ: $\pm 1^\circ\text{C}$ (35.0 - 37.0 $^\circ\text{C}$)

แบบประเมินผลการสอบเทียบเครื่องมือ

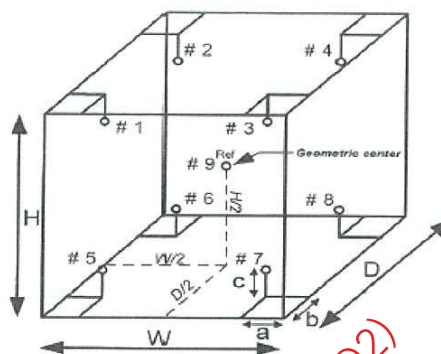


Figure: Example of sensor installation Positions

UUC Setting ($^\circ\text{C}$)	UUC Reading ($^\circ\text{C}$)	Calibration point [TS] ($^\circ\text{C}$)	Uncertainty [U] ($^\circ\text{C}$)	Position	Actual temp. [Ta] ($^\circ\text{C}$)	Error [E=Ta-Ts] ($^\circ\text{C}$)	E+U ($^\circ\text{C}$)	E-U ($^\circ\text{C}$)	เกณฑ์ MPE [E \pm U] $\leq \pm 1.0^\circ\text{C}$ Pass / Fail
35.80	35.80	36.00	0.33	1	36.00	0.00	0.33	-0.33	Pass
				2	36.13	0.13	0.46	-0.20	Pass
				3	36.08	0.08	0.41	-0.25	Pass
				4	36.08	0.08	0.41	-0.25	Pass
				5	36.19	0.19	0.52	-0.14	Pass
				6	36.10	0.10	0.43	-0.23	Pass
				7	36.12	0.12	0.45	-0.21	Pass
				8	35.99	-0.01	0.32	-0.34	Pass
				9	36.07	0.07	0.40	-0.26	Pass

ผลการสอบเทียบตู้ Incubator สามารถใช้งานได้ทุกตำแหน่ง

Error ($^\circ\text{C}$)	Correction Error x (-1) ($^\circ\text{C}$)	ช่วงการยอมรับ ($^\circ\text{C}$)	UUC Setting - [TS] ($^\circ\text{C}$)	ช่วงการใช้งานที่ยอมรับได้ ($^\circ\text{C}$)
Min	-0.01	0.0	35.0	34.8
Max	0.19	-0.2	37.0	36.6

ช่วงการทำงานของตู้ Incubator ที่ยอมรับได้อยู่ในช่วง 34.8 - 36.6 $^\circ\text{C}$

ผู้ตรวจ

Date: 25 OCT 2024

ผู้ตรวจ

Date: 29 OCT 2024

ผู้ตรวจ

Date: 29 OCT 2024

CERTIFICATE OF CALIBRATION

Page 1 of 3

Certificate No. : 24-111504

Sample Code : 24-44664-025

Customer : Betagro Science Center Co., Ltd.

Location of Calibration : Betagro Science Center Co., Ltd.
(Incubate)

Equipment : Temperature controlled enclosures (Incubator)

Manufacturer : HETTICH

Model : HettCube 400 R

Serial No. : 0000166-03

ID No. : B-IN-19

Date of Receipt : 02 September 2024

Date of Calibration : 02 September 2024

Condition of Calibration

1. Environment
- | | | | | |
|---------------------------|-----------|-----------|---------|-----------|
| 1.1 Ambient temperature | : Maximum | 26.3 °C | Minimum | 24.3 °C |
| 1.2 Relative humidity | : Maximum | 55.9 % | Minimum | 51.0 % |
| 1.3 Line voltage supplied | : Maximum | 229.4 VAC | Minimum | 225.7 VAC |

2. Calibration method

TLAS-G-20: Guidelines for calibration and checks of temperature controlled enclosures.

3. Reference standard instrument

Instrument	ID No.	Certificate No.	Due Date
Data Acquisition With Sensor (RTD-Pt100)	LB-DAMI (RTD-149, RTD-155, RTD-227)	24-040190	03 April 2025

4. This certificate is traceable to the international system of unit (SI Unit).

The measurement is traceable to Asia Medical and Agricultural Laboratory and Research Center Public Company Limited.

5. This result of calibration was found accurate as shown on date and place of calibration only.

6. Condition of calibration item : Normal

Calibrated by

Scientist

Approved by

Signed for Director

Issue date

06 September 2024

The uncertainties are for a confidence probability of approximately 95%.

The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Asia Medical and Agricultural Laboratory and Research Center Public Company Limited (AMARC).

REPORT OF CALIBRATION

Page 2 of 3

Certificate No. : 24-111504

Sample Code : 24-44664-025

Results of Calibration

Resolution : 0.1 °C

1. Reporting of Temperature

Calibration point (°C)	UUC* setting (°C)	UUC* reading (°C)	Measured temperature at each positions (°C)									Uncertainty ± (°C)	Coverage factor <i>k</i>
			# 1	# 2	# 3	# 4	# 5	# 6	# 7	# 8	# 9 ^{Ref}		
36	35.8	35.8	36.00	36.13	36.08	36.08	36.19	36.10	36.12	35.99	36.07	0.33	2.00

2. Characterization results

Calibration point (°C)	Stability ± (°C)	Uniformity (°C)	Overall variation (°C)
36	0.23	0.18	0.63

Notes

- UUC* = Unit Under Calibration

ใช้เพื่อประกอบเล่มรายงาน โครงการอาคารพักอาศัยแปลง D1 (อาคาร D2)
โครงการฟื้นฟูเมืองชุมชนดินแดง ระยะที่ 3
ฉบับประจำเดือนมกราคม - มิถุนายน 2568

REPORT OF CALIBRATION

Page 3 of 3

Certificate No. : 24-111504

Sample Code : 24-44664-025

Results of Calibration

Notes

1. Sensor installation locations
 - 1.1 All sensors at any corners or walls should be positioned 5 cm (a x b x c) from the wall.
 - 1.2 The reference sensor is preferably located of the geometric center of the chamber.
2. Interior dimensions approx of chamber :
W = 50 cm ; D = 60 cm ; H = 90 cm
3. Air valve or fresh air level : Off
4. Fan level : N/A
5. The quoted uncertainty includes " Stability of chamber and loading effect in chamber at 20% of uniformity ".
6. Uniformity - the maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time.
7. Stability - one-half of the greatest maximum difference of measured temperatures at any one sensor.
8. Overall variation - the difference of the maximum and the minimum measured temperatures throughout observation time.
9. UUC* reading - the average reading of indicating device that forms the integral part of the enclosure.
10. Calibration results without adjustment.

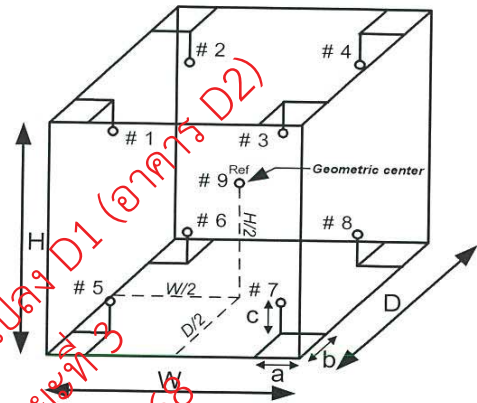


Figure: Example of sensor
installation Positions


The result expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k , which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty of measurement has been determined in accordance with UKAS M3003

- End of Report -



แบบประเมินผลการสอบเทียบเครื่องมือ

Instrument Name: Water bath
Manufacturer: Julabo
Model: ED
Serial No.: 10133832
ID No.: B-WB-05
Calibration Date: 3-Sep-24
Calibration by: สสท.
Certificate No.: 24TM1300
Temp Accept.: $44.5 \pm 0.2^{\circ}\text{C}$ (44.3 - 44.7 $^{\circ}\text{C}$)

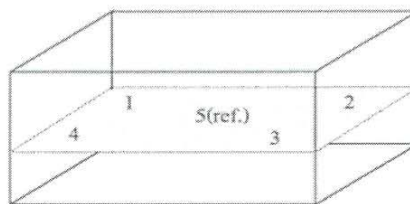

Front

ผลการประเมิน

UUC Setting ($^{\circ}\text{C}$)	UUC Reading ($^{\circ}\text{C}$)	Calibration point [TS] ($^{\circ}\text{C}$)	Uncertainty [U] ($^{\circ}\text{C}$)	Position	Actual temp. ($^{\circ}\text{C}$)	Error [E=Ta-Ts] ($^{\circ}\text{C}$)	E+U ($^{\circ}\text{C}$)	E-U ($^{\circ}\text{C}$)	เกณฑ์ MPE [E \pm U] $\leq \pm 0.2^{\circ}\text{C}$ Pass / Fail
45.10	45.10	44.50	0.15	1	44.497	-0.003	0.15	-0.15	Pass
				2	44.486	-0.014	0.14	-0.16	Pass
				3	44.493	-0.007	0.14	-0.16	Pass
				4	44.473	-0.027	0.12	-0.18	Pass
				5	44.473	-0.027	0.12	-0.18	Pass

ผลการสอบเทียบ เครื่อง Water bath สามารถใช้งานได้ ทุกตำแหน่ง

Error ($^{\circ}\text{C}$)	Correction Error x (-1) ($^{\circ}\text{C}$)	ช่วงการ ยอมรับ ($^{\circ}\text{C}$)	UUC Setting - 0 [TS] ($^{\circ}\text{C}$)	ช่วงการใช้งานที่ยอมรับได้ ($^{\circ}\text{C}$)
Min	-0.03	0.0	44.3	44.9
Max	0.00	0.0	44.7	45.3

ช่วงการทำงานของเครื่อง Water bath ที่ยอมรับได้อยู่ในช่วง (44.9 - 45.3 $^{\circ}\text{C}$)

ผู้จัดทำ..



Date..... 24 OCT 2024

ผู้ตรวจ..



Date..... 24 OCT 2024

ผู้ขอ..



Date..... 25 OCT 2024



Certificate of Calibration

Cert. No.: 24TM1300

Page : 1 of 3

Equipment : Water Bath
Manufacturer : Julabo
Model : ED
Serial No. : 10133832
ID No. : B-WB-05
Submitted by : Betagro Science Center Co., Ltd.

Location : Test #1 (No.104)

Received Order : 02 September 2024

Calibration Date : 03 September 2024

Ambient Temperature : $(26 \pm 10) ^\circ\text{C}$

Relative Humidity : $(50 \pm 30) \%$

Calibrated by : Tawatchai Pama

Approved by :

()

()

(✓)

Issue Date :

18 September 2024

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.



Equipment : Water Bath
Condition As-Received : Used Item
Reference : 2409-0002OC-1

Cert. No.: 24TM1300

Page : 2 of 3

Procedure Used :-

Calibration were conducted using in-house calibration procedure CP-OT04 Based on ASTM E715 according to direct measurement method with Data Acquisition which connected with Industrial Platinum Resistance Thermometer (IPRT).

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

<u>Instrument</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Traceable</u>	<u>Due Date</u>
1) Data Acquisition	MY49023932	24LM119	TPA	27 Jul 2025

2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certification is traceable to the International System of Unit.


Remark : TPA : Technology Promotion Association (Thailand - Japan)

Result of Calibration :- (*) Without Adjustment

Function of UUC* : Temperature Source

Heat transfer medium used : Water

	<u>Environmental</u>		<u>AC Voltage Supply</u>
	(°C)	%R.H.)	(Volt)
Beginning of Calibration	23	62	220
Finished of Calibration	23	62	221

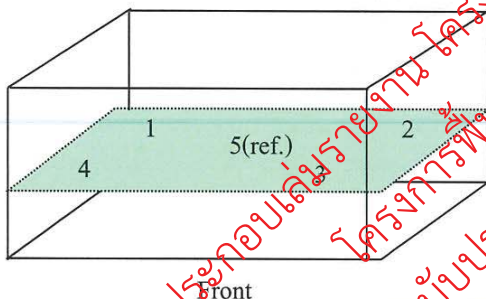

<u>Position :</u>	<u>Ref. Std. ID No.:</u>
1	70RC207
2	70RC208
3	70RC209
4	70RC352
5(ref.)	70RC353



Equipment : Water Bath
Condition As-Received : Used Item
Reference : 2409-0002OC-1
Result of Calibration :- (*) Without Adjustment
Function of UUC* : Temperature Source

Cert. No.: 24TM1300

Page : 3 of 3

Calibration point (°C)	UUC* Setting (°C)	UUC* Reading (°C)	Average* Standard Reading (°C)					Uncertainty (± °C)
			Position					
			1	2	3	4	5 (ref.)	
44.5	45.1	45.1	44.497	44.486	44.493	44.473	44.473	0.15

Calibration point (°C)	Uniformity (°C)	Stability (± °C)	Coverage Factor <i>k</i>
44.5	0.048	0.022	2

Average* : The average of 30 values in each position.

Uniformity : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.

Stability : One-half of the greatest maximum difference of measured temperature at any one probe.

UUC* : Unit Under Calibration

Note : The reported uncertainty of measurement was included stability and excluded uniformity.

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-