

ภาคผนวก ง

เอกสารการสอบเทียบเครื่องมือตรวจวิเคราะห์



Metrology

SCI ECO Services Company Limited

33/2 Moo 3, T. Banpa, A. Kaengkhoi, Saraburi 18110, Thailand.

Saraburi Tel : +66 3627 3096 Fax : +66 3627 3100

Bangkok Tel : +668 9205 6851 , +669 8247 2360

Website : www.scieco.co.th E-Mail : calibrate@scg.com



right solutions.
right partner.

รายการเครื่องมือที่ใช้ในการวิเคราะห์ / วัสดุ

Sample Name	Parameter	Equipment Name	ID No.	Calibrated Date	Next Cal	Freq. Calibrate (Months)
Water Lab	Fecal Coliform	Autoclave	BKK_IL0041	6-Mar-25	4-Sep-26	18
Water Lab	Fecal Coliform	Incubator	BKK_IL0010	3-Dec-24	3-Dec-25	12
Water Lab	Fecal Coliform	Hot Air Oven	BKK_IL0013	23-Apr-24	23-Oct-25	18
Water Lab	Fecal Coliform	Water Bath	BKK_IL0036	6-Mar-25	4-Mar-26	12
Water Lab	BOD	DO Meter	BKK_EN0026	2-Feb-24	24-Aug-25	18
Water Lab	BOD	Incubator	BKK_EN0072	22-Aug-24	22-Aug-25	12
Water Lab	BOD	Burette	BKK_EN0071	27-Feb-24	27-Aug-25	18
Water Lab	Oil & Grease	Electronic Top-Loading Balance	BKK_EN0003	24-Aug-24	24-Aug-25	12
Water Lab	Oil & Grease	Water Bath	BKK_EN0439	29-Oct-24	29-Oct-25	12
Water Lab	Oil & Grease	Hot meter	BKK_EN0342	11-Oct-24	11-Oct-25	12
Water Lab	Total Suspended Solids	Electronic Top-Loading Balance	BKK_EN0003	29-Aug-24	29-Aug-25	12
Water Lab	Total Suspended Solids	Oven	BKK_EN0273	14-Aug-24	14-Feb-25	18

alsglobal.com

1

Certificate No. T250353

Page 1 of 4

Certificate of Calibration

Equipment : Autoclave

Manufacturer : TOMY

Model : SX-700

Serial No. : 48134190

Customer Code : BKK_ML0041

ID No. : T7725A3

Customer : ALS Laboratory Group (Thailand) Co., Ltd.


104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan,

Khet Suan Luang, Bangkok 10250

Customer Location : Washing Room

Date of Receipt : 26 February 2025


Calibrated By : Boonchai Suriyawong (Site Calibration Manager)

Approved By :  / Sujjar Naknakred (Site Calibration Manager)

Date of Issue : 10 Mar 2025

The uncertainties are for a confidence probability of approximately 95%.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standard laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Metrology.





Metrology

SCI ECO Services Company Limited

33/2 Moo 3, T. Banpa, A. Kaengkhohi, Saraburi 18110, Thailand.



Certificate No. T250353

Page 2 of 4

Calibration Report

Equipment : Autoclave
Date of Calibration : 4 March 2025
Environment : Temperature : 22.2-25.4 °C
Line Voltage : 221.1-224.7 V
Relative Humidity : 55 - 65 %RH

Condition of this results of calibration :

1. This equipment was calibrated by insert 3 standard temperature recorder into its chamber and test according to WI-T23 inhouse method.(based on BS 2646-1 : 2021)
All data show below were final values and the initial data from customer request . The temperature scale used was based on ITS - 90 .

2. Reference Standard Instrument :

Instrument	Model	Standard No.	Certificate No.	Due Date
1. Temperature recorder	RTD	T210	T242028	11 December 2025
2. Temperature recorder	RTD	T211	T242029	11 December 2025
3. Temperature recorder	RTD	T212	T242030	11 December 2025

3. This certificate is traceable to :

National Institute of Metrology (Thailand) through Metrological Center (NSC-TIS-TIS 17025 CALIBRATION 0244.)

4. Condition of calibrated item : good

Equipment Description :

Pressure Indicator 0.11-0.12 MPa At 121 °C Holding time 20 minute

5. Adjustment :

(X) without adjustment

() after adjustment

Approved By. _____

FM-LJ5 118/18-08-66



Metrology

SCI ECO Services Company Limited


33/2 Moo 3, T. Banpa, A. Kaengkhohi, Saraburi 18110, Thailand.



Certificate No. T250353

Page 3 of 4

Calibration Report

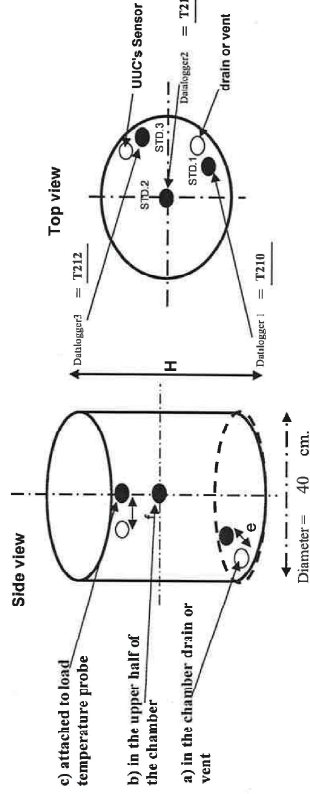

Remark :

Size of Installed Standard sensor STD.1 :Distance the chamber drain or vent e ≤ 10 cm.(less than or be equal to 10 cm.)

Size of Installed Standard sensor STD.2 :Geometric Center (upper half of the chamber)

Size of Installed Standard sensor STD.3 :Distance UUC's Sensor f = 2 cm.

Measurement Results :

Calibration Point	Average Standard Reading at each position (°C)	
	T210	T211
121	121.2	121.1

Setting (°C)	Autoclave		Temperature Distribution			
	Reading (°C)	Average (°C)	Stability (±°C)	Uniformity (±°C)	Uncertainty (±°C)	Coverage Factor k
121	Min, Max	Average	0.1	0.1	0.65	2.00

* The quoted uncertainty exclude "uniformity"

The calibration result apply only the above calibrated item.

The result of test was found accurate as shown on date and place of test only.

The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor k which for a t-distribution, providing a level of confidence of approximately 95 % .

End of Certificate

Approved By. _____

FM-LJ5 118/18-08-66



Metrological Center

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110

Telephone : +66 2 586 5792-4 Fax : +66 2 586 5109


Website : www.scieco.co.th E-Mail : calibrate@scg.co.th

Certificate No. T250353

TEST REPORT (BKK_ML0041)

Page 4 of 4

Calibration Report

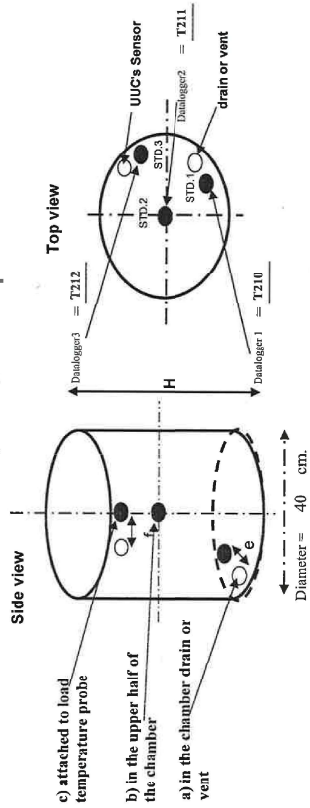

Remark :

Size of Installed Standard sensor STD.1 : Distance the chamber drain or vent $e \leq 10$ cm. (less than or be equal to 10 cm.)

Size of Installed Standard sensor STD.2 : Geometric Center (upper half of the chamber)

Size of Installed Standard sensor STD.3 : Distance UUC's Sensor $f = 2$ cm.

Measurement Results :

Calibration Point	Average Standard Reading at each position (°C)		
	T210	T211	T212
121	121.18	121.12	121.13

Autoclave		Temperature Distribution					
Setting (°C)	Reading (°C)		Average (°C)	Stability (± °C)	Uniformity (± °C)	Uncertainty (± °C)	Coverage Factor k
	Min.	Max					
121	-	121	121.16	0.10	0.10	0.65	2.00

* The quoted uncertainty exclude "uniformity"

The calibration result apply only the above calibrated item.

The result of test was found accurate as shown on date and place of test only.

The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor k which for a t-distribution, providing a level of confidence of approximately 95 % .

End of Certificate

Approved By.

FM-LJ13 108/30-05-57



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL 0-2717-3000-29 FAX 0-2719-9484



Certificate of Calibration

Cert. No.: 24TM1398

Page : 1 of 3

REVIEW BY	Sithichok T.
APPROVED BY	
NEXT CAL DATE	03/12/25

Equipment : Incubator
Manufacturer : SHEL-LAB
Model : 1915A
Serial No. : 0200599
ID No. : BKK_ML0010

Submitted by : ALS Laboratory Group (Thailand) Co.,Ltd.
104 Phatthanakan 40, Phatthanakan Rd.,
Khwaeng Phatthanakan, Khet Suan Luang,
Bangkok 10250 Thailand

Location : Incubation & Micrological Reading

Received Order : 03 December 2024
Calibration Date : 03 December 2024
Ambient Temperature : (26 ± 10) °C
Relative Humidity : (50 ± 30) %
AC Line Voltage : (220 ± 22) V

Calibrated by : Kunchit Promprat

Approved by : Approved Signatory

() Pornthippa Tameyakul
() Ponpan Paipim
(✓) Suwit Injai

Issue Date : 17 December 2024

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.



Equipment : Incubator
Condition As-Received : Used Item
Reference : 2412-0004OC-1

Cert. No.: 24TM1398
Page : 2 of 3

Procedure Used :-

Calibration were conducted using calibration procedure CP-OT02 based on TLAS G-20 according to direct measurement method with Data Acquisition which connected with Resistance Temperature Detector (RTD).
The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

Instrument **Serial No.** **Cert. No.** **Traceable** **Due Date**
1) Data Acquisition MY49023932 24LM119 TPA 27 Jul 2025


2. This certificate is valid only to the item calibrated on date and place of calibration.
3. This certification is traceable to the International System of Unit.

Remark : TPA : Technology Promotion Association (Thailand - Japan)

Result of Calibration :-

Function of UUC* : (*) Without Adjustment
Fresh air setting : Temperature Source
Close

Environment during calibration		
	Beginning	Finished
Temp. (°C)	24	24
REL.Humid. (%)	51	55
AC Supply (Volt)	223	223

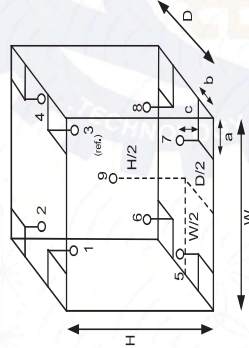

Probe Installation Details :

a = 10 cm
b = 10 cm
c = 10 cm

Dimension of Chamber :

D = 0.50 m
W = 0.75 m
H = 1.2 m
Capacity = 0.45 m³



Equipment : Incubator
Condition As-Received : Used Item
Reference : 2412-0004OC-1
Result of Calibration :- (*) Without Adjustment
Function of UUC* : Temperature Source
Fresh air setting : Close

Cert. No.: 24TM1398
Page : 3 of 3

Calibration Point (°C)	UUC* Setting (°C)	UUC* Reading (°C)	Temperature stability (± °C)	Temperature uniformity (°C)	Overall Variation (°C)	Coverage Factor k
35.0	35.0	35.0	0.048	0.40	0.46	2

Calibration Point (°C)	Measured Temperature (°C)									Uncertainty (± °C)
	Position									
	1	2	3	4	5	6	7	8	9 (ref.)	
	35.0	34.888	34.840	35.116	35.141	34.750	34.896	34.921	35.054	

Average* : The average of 30 values in each position.

Temperature stability : One-half of the greatest maximum difference of measured temperature at any one sensor.

Temperature uniformity : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.

Overall Variation : The Difference of the maximum and minimum measured temperatures throughout observation.

UUC* : Unit Under Calibration

Note : The reported uncertainty of measurement was included stability and excluded uniformity .

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor **k**, providing a level of confidence of approximately 95 %.

-o-o-



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
53/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL 0-2717-3000-29 FAX 0-2719-9484



Certificate of Calibration

Cert. No.: 24TM667
Page : 1 of 3

Equipment : Hot Air Oven
Manufacturer : Binder
Model : ED 240E2
Serial No. : 00-15533
ID No. : BKK_ML0013

Submitted by :

ALS Laboratory Group (Thailand) Co.,Ltd.
104 Phatthanakan 40, Phatthanakan Rd.,
Khwaeng Phatthanakan, Khet Suan Luang,
Bangkok 10250 Thailand
Media Preparation Room

Location :

Received Order : 23 April 2024
Calibration Date : 23 April 2024
Ambient Temperature : (26 ± 10) °C
Relative Humidity : (50 ± 30) %

Calibrated by :

Tawatchai Pama

Approved by :

() Ponpan Paipim
(✓) Suwit Imjai
() Kunchit Promprat

Approved Signatory

Issue Date :

26 April 2024

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.



Equipment : Hot Air Oven
Condition As-Received : Used Item
Reference : 2404-04390C-8
Procedure Used :-

Cert. No.: 24TM667
Page : 2 of 3

Calibration were conducted using calibration procedure CP-OT02 based on TLAS G-20 according to direct measurement method with Data Acquisition which connected with Thermocouple Type T.
The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

Instrument Serial No. Cert. No. Traceable Due Date
1) Data Acquisition MY49001451 24LM44 TPA 17 Mar 2025

2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certification is traceable to the International System of Unit.


Remark : TPA : Technology Promotion Association (Thailand - Japan)

Result of Calibration :- (*) Without Adjustment

Function of UUC* : Temperature Source

Fresh air setting : Close

Environment during calibration	
Temp. (°C)	Beginning 24 Finished 23
REL.Humid. (%)	65 65
AC Supply (Volt)	223 222

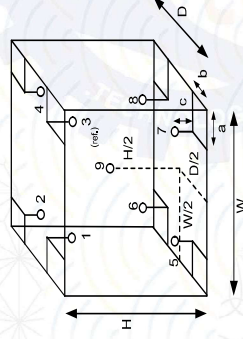

Probe Installation Details :

a = 10 cm
b = 10 cm
c = 10 cm

Dimension of Chamber :

D = 0.50 m
W = 0.80 m
H = 0.60 m
Capacity = 0.24 m³

Position :	Ref. Std. ID No.:
1	24-19TC-01
2	24-19TC-02
3	24-19TC-03
4	24-19TC-04
5	24-19TC-05
6	24-19TC-06
7	24-19TC-07
8	24-19TC-08
9 (ref.)	24-19TC-09



Equipment : Hot Air Oven
Condition As-Received : Used Item
Reference : 2404-0439OC-8
Result of Calibration :- (*) Without Adjustment
Function of UUC* : Temperature Source
Fresh air setting : Close

Cert. No.: 24TM667
Page : 3 of 3

Calibration Point (°C)	UUC* Setting (°C)	UUC* Reading (°C)	Temperature stability (± °C)	Temperature uniformity (°C)	Overall Variation (°C)	Coverage Factor k
180	180	180	0.64	2.7	3.7	2

Calibration Point (°C)	Measured Temperature (°C)									Uncertainty (±°C)
	1	2	3	4	5	6	7	8	9 (ref.)	
180	181.009	181.511	180.922	181.359	181.217	183.659	181.664	181.986	181.474	1.5

Average* : The average of 30 values in each position.

Temperature stability : One-half of the greatest maximum difference of measured temperature at any one sensor.

Temperature uniformity : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.

Overall Variation : The Difference of the maximum and minimum measured temperatures throughout observation.

UUC* : Unit Under Calibration

Note : The reported uncertainty of measurement was included stability and excluded uniformity .

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-000-



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL 0-2717-3000-29 FAX 0-2719-9484



Certificate of Calibration

Cert. No.: 25TM460
Page : 1 of 3

Equipment : Water Bath
Manufacturer : Memmert
Model : WNE 45
Serial No. : L712.0429
ID No. : BKK_ML0056

Submitted by : ALS Laboratory Group (Thailand) Co.,Ltd.
104 Phatthanakan 40, Phatthanakan Rd.,
Khwaeng Phatthanakan, Khet Suan Luang,
Bangkok 10250 Thailand
Location : Incubation & Microbiological Reading

Received Order : 04 March 2025
Calibration Date : 04 March 2025
Ambient Temperature : (26 ± 10) °C
Relative Humidity : (50 ± 30) %
AC Line Voltage : (220 ± 22) V

Calibrated by : Khit Ruttanaprapachai

Approved by : 
Approved Signatory

() Chakrit Waewwanjua
() Suwit Injai
(✓) Kunchit Promprat

Issue Date : 06 March 2025

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written approval of the head of Corporate Services 3: Equipment Calibration and Testing Services.



Equipment : Water Bath
Condition As-Received : Used Item
Reference : 2503-0006OC-2

Cert. No.: 25TM460
Page : 2 of 3

Procedure Used :-

Calibration were conducted using in-house calibration procedure CP-OT04 Based on ASTM E715 according to direct measurement method with Data Acquisition which connected with Industrial Platinum Resistance Thermometer (IPRT).

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

Instrument **Serial No.** **Cert. No.** **Traceable** **Due Date**
1) Data Acquisition MY44073381 23LM73 TPA 18 May 2025

2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certification is traceable to the International System of Unit.

Remark : TPA : Technology Promotion Association (Thailand - Japan)


Result of Calibration :-

(*) Without Adjustment

Function of UUC* : Temperature Source

Heat transfer medium used : Water

	Environmental		AC Voltage Supply
	(°C)	(%R.H.)	
Beginning of Calibration	24	49	220
Finished of Calibration	25	51	221

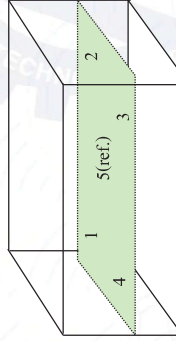

Front

Position :	Ref. Std. S/N.:
1	4803988-006
2	4803988-007
3	4804539-014
4	4804539-015
5(ref.)	4804539-016



Equipment : Water Bath
Condition As-Received : Used Item
Reference : 2503-0006OC-2
Result of Calibration :- (*) Without Adjustment
Function of UUC* : Temperature Source

Cert. No.: 25TM460
Page : 3 of 3

Calibration point (°C)	UUC* Setting (°C)	UUC* Reading (°C)	Average* Standard Reading (°C)					Uncertainty (± °C)
			1	2	3	4	5 (ref.)	
44.5	44.5	44.5	44.489	44.469	44.497	44.476	44.479	0.15
45.0	45.0	45.0	44.990	44.966	44.997	44.983	44.980	0.15

Calibration point (°C)	Uniformity (°C)	Stability (± °C)	Coverage Factor k
44.5	0.045	0.035	2
45.0	0.047	0.031	2

Average* : The average of 30 values in each position.

Uniformity* : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.

Stability* : One-half of the greatest maximum difference of measured temperature at any one probe.

UUC* : Unit Under Calibration

Note : The reported uncertainty of measurement was included stability and excluded uniformity.

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor **k**, providing a level of confidence of approximately 95 %.

-o0o-



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3 : EQUIPMENT CALIBRATION AND TESTING SERVICES

534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000 FAX. 0-2719-9484

Cert.No.: 24TW28
Page.: 1 of 2

Certificate of Testing

Equipment :	DO Meter
Manufacturer :	YSI
Model :	5100
Serial No. :	15L103204
ID No. :	BKK_EN0205
Received Date :	01 February 2024
Test Date :	02 February 2024
Reference :	2402-0008DSC-10
Submitted by :	ALS Laboratory Group (Thailand) Co.,Ltd. 104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan, Khet Suan Luang, Bangkok 10250 Thailand
Laboratory Condition :	Temperature (25 ± 5) °C Humidity (50 ± 20) % In - house method : CP-CH9 by Comparison Technique with Azide Modification Method
Test Procedure :	
Tested by :	Walalak Sirithean
Approved by :	Sathip Approved Signatory

(✓) Sathip Meangmai
() Warakorn Lengagtrakul
() Ponpan Paipim

Issue Date : 7 February 2024



Cert.No.: 24TW28
Page.: 2 of 2

Condition of this result of calibration

1. Reference Standard Instruments :

This certification is traceable to the International System of Unit through the reference standards laboratory of Industrial Calibration Center, Technology Promotion Association (Thailand-Japan).

Instruments	Serial No.	ID No.	Certificate No.	Due Date
1. Burette	-	130BU10	23CG1172	22 Mar 2025
2. Balance	1124013382	140RC006	23MM18	20 Feb 2024

2. Standard Material :-

Material	Manufacturer	Lot.No.	Assay
Sodium Thiosulfate pentahydrate	Merck	AM1763316	100.2%

Result : Dissolved Oxygen Meter Adjustment With Air 100 %
Dissolved Oxygen Probe No.: 17A100064

Titration Method (Azide Modification Method) (mg/L)	DO Meter Reading (mg/L)	Standard Deviation (mg/L)
8.18	8.18	0.0055

This report was certified only for the instrument we tested.It is allowable to use for study
Intend to use for advertising and referral purpose is prohibited.This report may not be reproduced
other in full,without written approval of the laboratory

-o0o-



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL.0-2717-3000-29 FAX.0-2715-9484



MSC185-1817023
CALIBRATION 0006

Certificate of Calibration

Cert. No.: 24LM15
Page.: 1 of 2

Equipment : DO Meter with Sensor
Manufacturer : YSI
Model : 5100
Serial No. : 15L103204
ID No. : BKK_EN0205
Submitted by : ALS Laboratory Group (Thailand) Co.,Ltd.
104 Phatthanakan 40, Phatthanakan Rd.,
Khuwaeng Phatthanakan, Khet Suan Luang,
Bangkok 10250 Thailand
Location : TPA Chemistry Calibration Laboratory
Received Order : 01 February 2024
Calibrated Date : 02 February 2024
Ambient Temperature : (26 ± 10) °C
Relative Humidity : (50 ± 30) %
AC Line Voltage : (220 ± 22) V

Calibrated by : Warakorn Lengagtrakul

Approved by : 
Approved Signatory

() Ponthippa Tameyakul
() Ponpan Paipim
(✓) Suwit Imjai

Issue Date : 7 February 2024

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the Head of Corporate Services 3 : Equipment Calibration and Testing Services.



Equipment : DO Meter with Sensor
Condition As-Received : Used Item
Reference : 2402-0008DSC-13
Procedure Used :-

Calibration were conducted using in-house calibration procedure CP-OT01 according to comparison with
Industrial Platinum Resistance Thermometer (IPT) into Temperature Bath.
The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

Instrument **Serial No.** **Cert. No.** **Traceable** **Due Date**
1) Digital Thermometer 2188080 231216 TPA 11 Oct 2024

2. This certificate is valid only to the item calibrated on date and place of calibration.
3. This certification is traceable to the International System of Unit.

Remark : TPA : Technology Promotion Association (Thailand - Japan)

Result of Calibration :- (*) Without Adjustment

Function : Temperature measurement.

This instrument was connected with temperature sensor, S/N.: 17A100064

Calibration Point (°C)	Immersion Depth (mm)	Standard Temperature (°C)	UUC* Reading (°C)	Error (°C)	Uncertainty (± °C)	Coverage Factor k
20.0	80	20.003	19.92	-0.083	0.15	2.00

UUC* : Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor **k**, providing a level of confidence of approximately 95 %.

-o-o-



Metrology

SCI ECO Services Company Limited

33/2 Moo 3, T. Banpa, A. Kaengkhohi, Saraburi 18110, Thailand.

Saraburi Tel : +66 3627 3096 Fax : +66 3627 3100

Bangkok Tel : +668 9205 6851, +669 8247 2360

Website : www.scieco.co.th E-Mail : calibrate@scg.com



NSC-TISI-TIS 17025
CALIBRATION 0244

Certificate No. T241495

Page 1 of 4

Certificate of Calibration

Equipment : Chamber (Incubator)

Manufacturer : MEMMERT

Model : ICP 750

Serial No. : F818.0033

Customer Code : BKK_EN0272

ID No. : T8041A4

Customer : ALS Laboratory Group (Thailand) Co.,Ltd.

104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan,

Khet Suan Luang, Bangkok 10250

Customer Location : Wet Chemistry Lab 2

Date of Receipt : 14 August 2024

Calibrated By : Sujjar Naknakred (Site Calibration Manager)

Approved By :  / Boonchai Suriyawong (Assistant Calibration Manager)

Date of Issue : 17 AUG 2024

The uncertainties are for a confidence probability of approximately 95%.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standard laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Metrology.

FM-L14.119/18-08-66



Metrology

SCI ECO Services Company Limited

33/2 Moo 3, T. Banpa, A. Kaengkhohi, Saraburi 18110, Thailand.



NSC-TISI-TIS 17025
CALIBRATION 0244

Certificate No. T241495

Page 2 of 4

Calibration Report

Equipment : Chamber (Incubator)
Date of Calibration : 22 August 2024 (Finished Time 11:19 AM)
Environment : Temperature 22.3-23.0 °C
Line Voltage 222.5-227.5 V

Condition of this results of test. :

1. This instrument was calibrated by insert 12 standard resistance thermometer into its chamber and test according to WI-T20 (based on ASTM E145-94 (Reapproved 2001) and AS2853-1985.)
All data show below were final values and the initial data may be obtained upon request.

The temperature scale used was based on ITS - 90.

2. Reference Standard Instrument :

Instrument	Model	Instrument No.	Certificate No.	Due Date
RTD	100 ohm	27-(CH1-10)	T240709	19 April 2025
RTD	100 ohm	28-(CH1-10)	T240709	19 April 2025
DATA LOGGER	34970A	T149	T240709	19 April 2025

3. This certificate is traceable to :

National Institute of Metrology (Thailand) through Metrological Center (NSC-TISI-TIS 17025 CALIBRATION 0244.)

4. Condition of calibrated item : good

UUC Description :

Time Constant 1 Hour 38 Minute At 20 °C
Fresh Air Damper ☐ Open ☐ Min ☐ Medium ☐ Max
☐ Close ☒ Not Available

5. Result of test :

() without adjustment (X) after adjustment

Approved By: 

FM-L15.118/18-08-66



Metrology

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110, Thailand.




NSC-TIS-TIS 17025
CALIBRATION 0244

Certificate No T241495

Page 3 of 4

Calibration Report

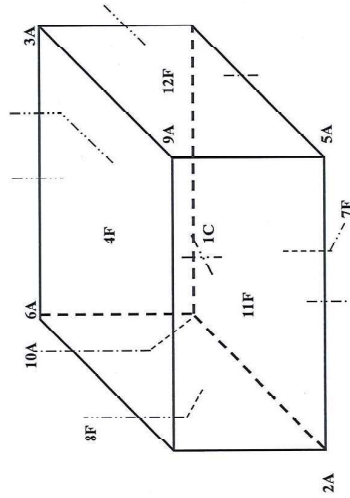

C = Centre, F = Centre of Face, A = Corner, E = Centre of Edge

1C	=	27-CH1
2A	=	27-CH2
3A	=	27-CH3
4F	=	27-CH4
5A	=	27-CH5
6A	=	27-CH6
7F	=	27-CH7
8F	=	27-CH8
9A	=	27-CH9
10A	=	27-CH10

11F	=	28-CH1
12F	=	28-CH2

Approved By. 

FM-L15 118/18-03-66



Metrology

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110, Thailand.



NSC-TIS-TIS 17025
CALIBRATION 0244

Certificate No. T241495

Page 4 of 4

Calibration Report

Measurement Results

Calibration Point	Average Standard Reading at each position (°C)									
	27-CH1	27-CH2	27-CH3	27-CH4	27-CH5	27-CH6	27-CH7	27-CH8	27-CH9	27-CH10
20.0	20.32	20.32	20.29	20.23	20.30	20.34	20.40	20.16	20.34	19.62
	28-CH1	28-CH2								
	19.70	19.65								

Chamber(Incubator)			Temperature Distribution					Coverage Factor k
Setting (°C)	Reading (°C)		Average (°C)	Stability (± °C)	Uniformity (°C)	Uncertainty (± °C)		
	Min, Max	Average						
20.0	19.9, 20.1	20.0	20.01	0.04	0.19	0.38	2.00	

* The quoted uncertainty exclude "uniformity"

The calibration result apply only the above calibrated item.

The result of test was found accurate as shown on date and place of test only.

The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor k which for a t-distribution, providing a level of confidence of approximately 95 %.

Approved By. 

FM-L15 118/18-03-66



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANA KAFEN ROAD SOI 16, SUANLUANG, SUANLUANG BANGKOK 10250
TEL.0-2717-3000-29 FAX.0-2719-9484



Certificate of Calibration

Cert.No.: 24CG952
Page.: 1 of 2

Equipment : Burette
Capacity : 50 mL
Serial No. :
ID. No. : BKK_EN0171
Manufacturer : Witeg
Made in : Germany

Submitted by : ALS Laboratory Group (Thailand) Co.,Ltd.
104 Phatthanakan 40, Phatthanakan Rd.,
Khwaeng Phatthanakan, Khet Suan Luang,
Bangkok 10250 Thailand

Ambient Temperature : $(20 \pm 2.5) ^\circ\text{C}$
Relative Humidity : $(50 \pm 10) \%$
Barometric Pressure : 760 mmHg
Calibration Procedure : ASTM E 542 - 01

Calibrated by : Natcha Chayingcheiw

Approved by :
() Unnophol Harachai
(✓) Srisuda Khamtha
() Sa-ngeunkam Wongs

Issue Date : 27 February 2024

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 - Equipment Calibration and Testing Services.



Equipment : Burette
Received Date : 23 February 2024
Condition As-Received : New Item
Calibration Date : 27 February 2024
Reference : 2402-0757DSC-1

Cert.No.: 24CG952
Page.: 2 of 2

Condition of this result of calibration

1. Reference Standard Instruments :

Instruments	Model	Serial No.	ID. No.	Certificate No.	Traceability	Due date
1) Balance	XP205DR	1126143764	140RC004	23MM538	TPA	15 Sep 2024
2) Thermo-Hygograph	THDX-CE	00016540	140EC001	23H1275	TPA	09 June 2024
3) Thermometer	-	0834181	140EC005	23I948	TPA	10 Aug 2024

This certification is traceable to SI Unit

2. The certificate is valid only to the item calibrated on date and place of calibration.

3. True value is converted to true volume at the standard temperature of $20 ^\circ\text{C}$

Calibration result :

Nominal capacity (mL)	Reading (mL)	Uncertainty (\pm mL)	k Factor
50	50.0032	0.010	2.00

Remark: mL = cm³

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k , providing a level of confidence of approximately 95 %.

-o0o-

Sartorius (Thailand) Co., Ltd.
129 Rama 9 Road, Huaykwang, Bangkok 10310
Tel: +66 2643 8861-6, e-mail: service.thailand@sartorius.com



NSC-TIS-17025
CALIBRATION 0426

REVIEW BY: Junda K
APPROVED BY: Siluk P
NEXT CAL DATE: 02/08/25

SARTORIUS

Certificate

of Calibration

Model Number: MSE224S-100-DU
Description: Analytical Balance
Serial Number: 0027405555
ID No.: BKK-EN0003
Manufacturer: Sartorius

Certificate No.: 24BCI0270
Issued Date: Monday, August 05, 2024
Reference No.: 240942
Page No.: 1 of 2

Customer Name: ALS Laboratory Group (Thailand) Co., Ltd.
104 Phatthanakan 40/Phatthanakan Rd., Kiwaeng Suan Luang, Khet Suan Luang, Bangkok 10250.

Calibrated Place: Lab Room

Calibrated By: Mr.Chonchai Inthana
Calibration Date: Friday, August 02, 2024

Calibration Procedure No.: This calibration was conducted by
Using in-house calibration procedure number (WI-003)
Based on UKAS IAB 14 : 2019

Metrological data :
Capacity: 220 g Readability: 0.0001 g Temperature: 23.0 °C ± 5.0 °C
Humidity: 55.0 % RH ± 10.0 % RH
Pressure: ±

Reasons for calibration
☐ New installation ☐ Service / Repaired ☒ Re-calibration/ Maintenance ☐ Good Operation ☐ Fail

Measurement Method UKAS Publication Ref :Lab 14

The measurement uncertainty stated is the expanded uncertainty which is obtained from the standard uncertainty multiplied by the coverage factor (k=2) to provide a level of confidence of approximately 95%. It is determined in accordance with the Guide to Expression of Uncertainty in Measurement (GUM). The calibration certificate documents the traceability to National Standards, which realise the unit of measurement according to the International Standard System of Units (SI). Report of Tolerance came from list of Sartorius Metrological Specifications.

Traceability:

Model Number	Description	Traceability	Certificate No.	Due Date
YCS011-522-00	Sartorius weight set 1mg - 5000g E2/YS011-522-00	TCS	M73081975	23-Aug-2025
Testo 174 H	Thermo-Hygrometer, Testo 174H	ENTECH	HJT 661303;H661140	12-Nov-2024

This certificate relate and apply this equipment only.
This certificate may not be reproduced other than in full except with the prior written approval of the Verification Operation Division Sartorius (Thailand) Co., Ltd.

Mr.Chonchai Inthana(Technical Manager)



Sartorius (Thailand) Co., Ltd.
129 Rama 9 Road, Huaykwang, Bangkok 10310
Tel: +66 2643 8861-4 Fax: +66 2643 8357, e-mail: service.thailand@sartorius.com

Sartorius (Thailand) Co., Ltd.

Certificate

of Calibration

Model Number: MSE224S-100-DU
Description: Analytical Balance
Serial Number: 0027405555
ID No.: BKK-EN0003
Manufacturer: Sartorius

Certificate No.: 24BCI02710
Issued Date: Monday, August 05, 2024
Reference No.: 240942
Page No.: 2 of 2

Calibration Results : Without Adjustment

Repeatability			Eccentricity (Off-center loading error)		
The repeatability is the ability of a weighing instrument to display nearly identical results under constant test conditions when the same load within a measurement series is placed repeatedly on the weighing pan in the same manner. The standard deviation is used to express reproducibility quantitatively.			The off-center loading error is visible for the difference between the measure of the load, i.e. 1/3 or 1/4 of maximum capacity, placed in the middle of the weighing pan and between each of four additional measurement points (positions defined according to OIML R110).		
Nominal Value (Low Load)	20.0000	203.0000	Nominal value:	100	g
20 g	20.0000	199.9999	Tolerance	0.0004	g
Tolerance	0.0001	203.0000	Difference		
		20.0000	1	0.0000	
		20.0000	2	0.0000	
		20.0000	3	0.0000	
		20.0000	4	0.0000	
		20.0000	5	0.0001	
		20.0000	6	-	
Nominal Value (High Load)	20.0000	203.0000			
200 g	20.0000	203.0001			
Tolerance	0.0001	203.0000			
		199.9999			
		203.0000			
Standard Deviation	0.00004	0.00006			

Linearity

The linearity, also called linearity error, describes the deviation of the characteristic curve of a weighing instrument from the linear slope.

Tolerance 0.0002 g

Nominal Value (g)	Conventional Mass Value (g)	Displayed Value (g)	Deviation (g)	Uncertainty (g)
0.01	0.0100	0.0100	0.0000	0.00015
0.1	0.1000	0.1000	0.0000	0.00015
1	1.0000	1.0000	0.0000	0.00015
2	2.0000	2.0000	0.0000	0.00015
5	5.0000	5.0000	0.0000	0.00015
10	10.0000	10.0000	0.0000	0.00015
20	20.0000	20.0000	0.0000	0.00015
50	50.0000	50.0001	0.0001	0.00016
100	100.0000	100.0001	0.0001	0.00019
200	200.0000	200.0000	0.0000	0.00029

End of Report.



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
E34/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL 0-2717-3000-29 FAX 0-2719-9484



Certificate of Calibration

Cert. No.: 24TM1618
Page : 1 of 3

Equipment : Water Bath

Manufacturer : Memmert

Model : WNE29

Serial No. : L622.0282

ID No. : BKK_EN0439

Submitted by : ALS Laboratory Group (Thailand) Co.,Ltd.
104 Phatthanakan 40, Phatthanakan Rd.,
Khwaeng Phatthanakan, Khet Suan Luang,
Bangkok 10250 Thailand

Location : Organic Preparation Lab

Received Order : 29 October 2024

Calibration Date : 29 October 2024

Ambient Temperature : (26 ± 10) °C

Relative Humidity : (50 ± 30) %

Calibrated by : Man Pattanapongpalboon

Approved by : 
Approved Signatory

() Ponpan Palpim
() Suwit Imjai
(✓) Kunchit Promprat

Issue Date : 30 October 2024

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.



Equipment : Water Bath
Condition As-Received : Used Item
Reference : 2410-0782OC-4
Page : 2 of 3

Procedure Used :-

Calibration were conducted using in-house calibration procedure CP-OT04 Based on ASTM E715 according to direct measurement method with Data Acquisition which connected with Industrial Platinum Resistance Thermometer (IPT).

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

Instrument Serial No. Cert. No. Traceable Due Date
1) Data Acquisition MY57013711 24LM115 TPA 13 Jul 2025

2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certification is traceable to the International System of Unit.


Remark : TPA : Technology Promotion Association (Thailand - Japan)

Result of Calibration :- (*) Without Adjustment

Function of UUC* : Temperature Source

Heat transfer medium used : Water

	Environmental		AC Voltage Supply (Volt)
	(°C)	(%R.H.)	
Beginning of Calibration	25	54	222
Finished of Calibration	25	57	226

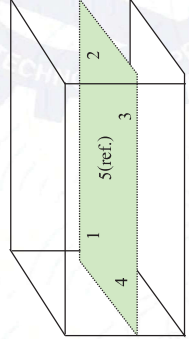

Front

Position :	Ref. Std. ID No.:
1	4803988-001
2	4803988-002
3	4803988-003
4	4803988-004
5(ref.)	4803988-005



Equipment : Water Bath
Condition As-Received : Used Item
Reference : 2410-0782OC-4
Result of Calibration :- (*) Without Adjustment
Function of UUC* : Temperature Source

Cert. No.: 24TM1618
Page : 3 of 3

Calibration point (°C)	UUC* Setting (°C)	UUC* Reading (°C)	Average* Standard Reading (°C)					Uncertainty (± °C)
			1	2	3	4	5 (ref.)	
85.0	85.0	85.0	85.133	85.212	85.150	84.983	85.096	0.22

Calibration point (°C)	Uniformity (°C)	Stability (± °C)	Coverage Factor <i>k</i>
85.0	0.21	0.13	2

Average* : The average of 30 values in each position.
Uniformity : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.
Stability : One-half of the greatest maximum difference of measured temperature at any one probe.
UUC* : Unit Under Calibration
Note : The reported uncertainty of measurement was included stability and excluded uniformity.

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANILUANG, SUANLUANG BANGKOK 10250
TEL.0-2717-3000-26 FAX.0-2719-9484



MSC185-187:2025
CALIBRATION 0004

Certificate of Calibration

Cert.No.: 24CH1295
Page.: 1 of 3

Equipment : pH Meter
Manufacturer : Hach
Model : HQ411d
Serial No. : 200100031163
ID No. : BKK_EN0342
Condition As-Received: Used Item
Received Date : 16 October 2024
Calibration Date : 17 October 2024
Reference : 2410-0548DSC-5
Submitted by : ALS Laboratory Group (Thailand) Co.,Ltd.
104 Phatthanakan 40, Phatthanakan Rd.,
Khaewang Phatthanakan, Khet Suan Luang,
Bangkok 10250 Thailand

Ambient Temperature : (25 ± 2.5) °C
Relative Humidity : (50 ± 15) %
Calibration Procedure : In - house method :
- CP-CH5 by direct measurement with certified reference material (CRM)
- CP-CH8 by comparison with temperature standard

Calibrated by : Warakorn Lergagatrakul

Approved by : *Saithip*
Approved Signatory

() Unnoppol Harachai
() Ponpan Paipim
(✓) Saithip Meangmai

Issue Date : 21 October 2024

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.



Cert.No.: 24CH1295
Page.: 2 of 3

Condition of this calibration result

- Reference Standard Instrument

Instrument	Serial No.	ID No.	Cert. No.	Due Date
1) Ref. Standard Thermometer	2188080	130RC044	2411022	16 Sep 2025
- This Certification is traceable to SI Through Technology Promotion Association (Thailand - Japan)
- Certified Reference Materials
:The measurement results are traceable to SI through Hach Lange GmbH Ltd.
Deutsche Akkreditierungsstelle, Accredited No.D-RM-15184-01-00
:The measurement results are traceable to SI through CPA chem Ltd.,
ANSI-ASQ National Accreditation Board, Accredited No. AR-1835

Buffer Solution	Manufacturer	Lot No.	Exp. date
pH 4.008	CPA chem	1034203	27 Sep 2026
pH 6.999	Hach Lange GmbH	C03145	28 Feb 2026
pH 10.010	CPA chem	1034205	27 Sep 2025

- This certificate is valid only to the item calibrated on date and place of calibration.

Calibration Results

Function : pH Measurement

Performing three buffers standard curve by using buffer nominal pH (4,7,10)

Unit Under Calibration	Standard pH Buffer Solution	Actual pH Reading	Actual mV Reading (mV)	Uncertainty of pH Measurement (±)	Coverage factor k
pH Electrode S/N.: 230473042902	4.008	4.028	174.6	0.0044	2.00
	6.999	7.014	1.4	0.0084	2.05
	10.010	10.018	-172.8	0.0066	2.00

Remark - Can not connect the BNC because the plug does not match with the socket.



Cert.No.: 24CH1295
Page.: 3 of 3

Calibration Results

Function : Temperature Measurement

(*) Without adjustment

This equipment was connected with Temperature Probe;


- Model : PHC281
- Serial No. : 230473042902
Dimension of probe
- Length : 103 mm.
- Diameter : 12 mm.
- Immersion Depth : 90 mm.

Calibration Point (°C)	Standard Temperature (°C)	UUC* Reading (°C)	Error (°C)	Uncertainty of measurement (± °C)	Coverage factor k
25.0	25.002	25.0	-0.002	0.13	2.00

Remark : UUC* = Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k , providing a level of confidence of approximately 95 %.

-o0o-



Metrology

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110, Thailand.

Bangkok Tel : +66 3627 3096 Fax : +66 3627 3100

Banpakong Tel : +668 9205 6851, +669 8247 2360

Website : www.scieco.co.th E-Mail : calibrate@scg.com



Certificate No. T240904

Page 1 of 3

Certificate of Calibration

Equipment : Chamber (Oven)
Manufacturer : Memmert
Model : UF 450
Serial No. : B717.0531
Customer Code : BKK_EN0273
ID No. : T8042A4
Customer : ALS Laboratory Group (Thailand) Co.,Ltd.

104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan,

Khet Suan Luang, Bangkok 10250

Customer Location : Laboratory (Oven Room)

Date of Receipt : 08 May 2024

Calibrated By : Preecha Phisassuthikul (Temperature Calibration Manager)


Approved By : / Nuafun Sungchum (Metrology Manager)

Date of Issue : 23 MAY 2024

The uncertainties are for a confidence probability of approximately 95%.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standard laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Metrology.

FM-L14 119/18-08-66



Metrology

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110, Thailand.



Certificate No. T240904

Page 2 of 3

Calibration Report

Equipment : Chamber (Oven)
Date of Calibration : 14 May 2024
Environment : Temperature : 26.5-28.1 °C
Line Voltage : 226.7-229.8 V
Relative Humidity : 51 - 57 %RH

Condition of this results of calibration :

1. This equipment was calibrated by insert nine resistance thermometer detectors into its chamber, the other one resistance thermometer detector use for ambient temperature measurement. The calibration was done in according to WI-T20 (based on ASTM E145-94 (Reapproved 2001) and AS2853-1986).

All data show below were final values and the initial data from customer request. The temperature scale used was based on ITS - 90.

2. Reference Standard Instrument :

Instrument	Model	Instrument No.	Certificate No.	Due Date
RTD	100 ohm	21-(CHI-10)	T231955	17 November 2024
DATA LOGGER	34970A	T121	T231955	17 November 2024

3. This certificate is traceable to :

National Institute of Metrology (Thailand) through Metrological Center (NSC-TISI-TIS 17025 CALIBRATION 0244.)

4. Condition of calibrated item : good


Equipment Description :

Time Constant : 1 Hour 30 Minute At 104 °C
Fresh Air Damper : ☐ Open ☐ Min ☐ Medium ☐ Max
☐ Close ☒ Not Available

5. Adjustment : (X) without adjustment () after adjustment

Approved By :

FM-L15 118/18-08-66



Metrology

SCI ECO Services Company Limited

33/2 Moo 3, T. Banpa, A. Kaengkhroi, Saraburi 18110, Thailand.




NSC-TIS-TIS 17025
CALIBRATION 0244

Certificate No. T240904

Page 3 of 3

Calibration Report

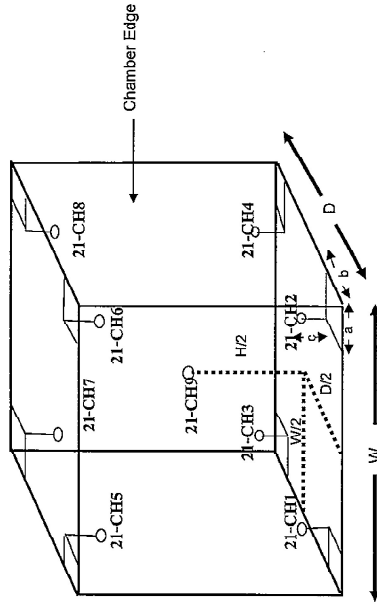

Remark :

Internal Dimensions of Chamber : W (Width) = 104 cm. , H(Height)=72 cm. and D(Depth)=60 cm.
Size of Installed Standard sensor number 21-CH1 to number 21-CH8 : a = 5 cm. b = 5 cm. and c = 5 cm.
Size of Installed Standard sensor number 21-CH9 : W/2=104 cm./2 , H/2=72 cm./2 and D/2=60 cm./2

Measurement Results

Calibration Point	Average Standard Reading at each position (°C)								
	21-CH1	21-CH2	21-CH3	21-CH4	21-CH5	21-CH6	21-CH7	21-CH8	21-CH9
104	103.4	103.0	103.7	103.6	103.3	104.6	103.3	104.0	103.9
180	179.5	181.1	179.2	179.5	179.0	181.3	179.8	179.9	180.2

Chamber (Oven)		Temperature Distribution					Coverage Factor k
		Reading (°C)	Average (°C)	Stability (± °C)	Uniformity (°C)	Uncertainty (± °C)	
		Min, Max	Average				
104.0		103.9 , 104	104.0	0.14	1.27	0.44	2.00
180.0		179.9 , 180.1	180.0	0.39	2.29	0.76	2.00

* The quoted uncertainty exclude "uniformity"

The calibration result apply only the above calibrated item.

The result of test was found accurate as shown on date and place of test only.

The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor k which for a t-distribution, providing a level of confidence of approximately 95 % .

End of Certificate

Approved By: