

ภาคผนวก 7-1

สำเนา ใบสอบเทียบเครื่องมือตรวจวัด
และวิเคราะห์

PM10 Sampler Calibration

SITE

Project: High Volume Sampler Calibration
Location: Life & Environment Co., Ltd
Date of calibration : February 14, 2024

DETAIL OF SAMPLER

Sampler Model: TE-6070 PM-10
Motor Model: TISCH
Motor Serial No.: 2184

CONDITIONS

Pressure of Ambient Air (Pa) (mm Hg):	760
Temperature of Ambient Air (Ta) (K):	305
Average Pressure (Ps) (mm Hg):	759
Average Temperature (Ts) (K):	302

CALIBRATION ORIFICE

Make : Tisch	Slope :	1.26202
Model : TE-5025A	Intercept:	-0.01176
Serial#: 5		

CALIBRATION

Plate or Test #	H ₂ O (in)	Qa (m ³ /min)	I (chart)	IC (corrected)	LINEAR REGRESSION
1	11.40	1.704	54.0	34.21	Slope = 18.9651
2	9.60	1.565	48.0	30.41	Intercept = 1.0675
3	7.50	1.384	42.0	26.61	Corr. coeff. = 0.9951
4	4.70	1.098	34.0	21.54	SFR = 1.140
5	2.80	0.849	28.0	17.74	SSP = 37.75

of Observations: 5

Calibrated by:



Approved by :



Industrial Hygiene Specialist

PM10 Sampler Calibration

SITE

Project: High Volume Sampler Calibration
Location: Life & Environment Co., Ltd
Date of calibration: February 14, 2024

DETAIL OF SAMPLER

Sampler Model: TE-6070 PM-10
Motor Model: TISCH
Motor Serial No.: 2095

CONDITIONS

Pressure of Ambient Air (Pa) (mm Hg): 760
Temperature of Ambient Air (Ta) (K): 305
Average Pressure (Ps) (mm Hg): 759
Average Temperature (Ts) (K): 302

CALIBRATION ORIFICE

Make : Tisch Slope : 1.26202
Model : TE-5025A Intercept: -0.01176
Serial#: 5

Plate or Test #	H ₂ O (in)	Qa (m ³ /min)	CALIBRATION		LINEAR REGRESSION
			I (chart)	IC (corrected)	
1	11.50	1.712	58.0	36.74	Slope = 21.2408 Intercept = 0.2203 Corr. coeff. = 0.9957 SFR = 1.140 SSP = 37.75
2	9.50	1.556	52.0	32.94	
3	6.90	1.328	46.0	29.14	
4	4.80	1.109	36.0	22.81	
5	2.90	0.864	30.0	19.00	

of Observations: 5

Calibrated by:



Approved by :



Industrial Hygiene Specialist

PM10 Sampler Calibration

SITE

Project: High Volume Sampler Calibration
Location: Life & Environment Co., Ltd
Date of calibration: February 14, 2024

DETAIL OF SAMPLER

Sampler Model: TE-6070 PM-10
Motor Model: TISCH
Motor Serial No.: 2094

CONDITIONS

Pressure of Ambient Air (Pa) (mm Hg):	760
Temperature of Ambient Air (Ta) (K):	305
Average Pressure (Ps) (mm Hg):	759
Average Temperature (Ts) (K):	302

CALIBRATION ORIFICE

Make : Tisch	Slope :	1.26202
Model : TE-5025A	Intercept:	-0.01176
Serial#: 5		

Plate or Test #	H ₂ O (in)	Qa (m ³ /min)	CALIBRATION		LINEAR REGRESSION
			I (chart)	IC (corrected)	
1	11.50	1.712	52.0	32.94	Slope = 21.9130 Intercept = -4.4403 Corr. coeff. = 0.9997 SFR = 1.140 SSP = 37.75
2	9.20	1.532	46.0	29.14	
3	7.20	1.356	40.0	25.34	
4	4.60	1.086	31.0	19.64	
5	2.80	0.849	22.0	13.94	

of Observations: 5

Calibrated by:

(M)

Approved by :

Industrial Hygiene Specialist

CALIBRATION TEST REPORT

Instrument : AIR CHECK SAMPLER (Low Flow)

Serial No. 038536

Model : 224-PC X R8


Manufacture : SKC (INC)

Date of Calibration : MARCH 11, 2024


AM-15

Next Time Calibration : MARCH 11, 2025


Standard Criteria : Rota Meter					Ambient Condition		
SKC Model1355EZ30 S/N 0107070345011/003					Temperature = 25.0 °C		
					Pressure = 759 mmHg		
Rota Meter Reading	Actual Flow Rate (l/min)				Deviation (l/min)	Permissible Deviation (l/min)	Status
	1	2	3	Average			
0.01	0.01	0.01	0.01	0.010	0.0000	±0.05	Pass
0.05	0.05	0.04	0.04	0.043	0.0058	±0.10	Pass
0.10	0.12	0.10	0.10	0.107	0.0115	±0.15	Pass
0.20	0.19	0.19	0.20	0.193	0.0058	±0.20	Pass

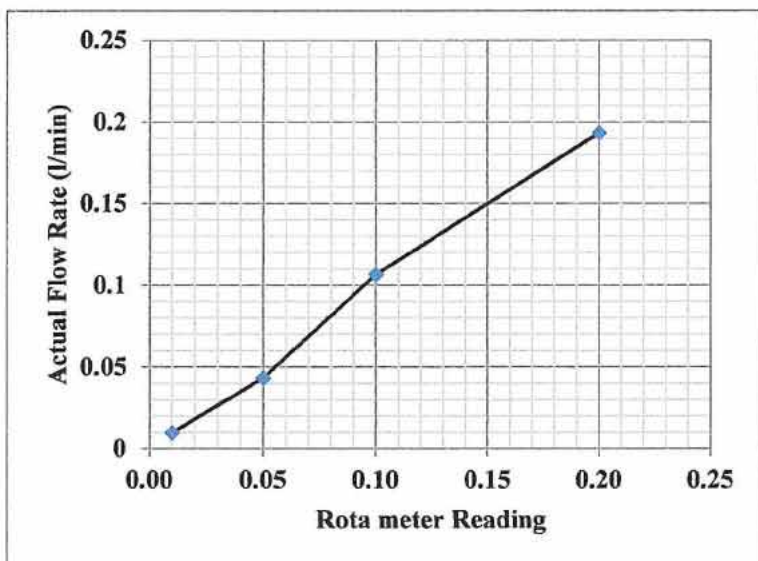

Calibrated by

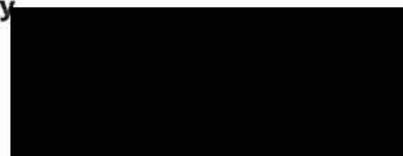

Approved by

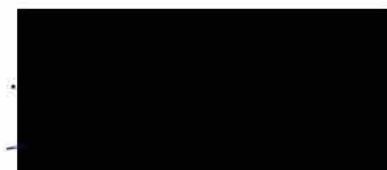

Industrial Hygiene Specialist

CALIBRATION TEST REPORT

Instrument : AIR CHECK SAMPLER (Low Flow)

Serial No. 038556

Model : 224-PC X R8


Manufacture : SKC (INC)

Date of Calibration : MARCH 11, 2024

AM-16

Next Time Calibration : MARCH 11, 2025

Standard Criteria : Rota Meter					Ambient Condition		
SKC Model1355EZ30 S/N 0107070345011/003					Temperature = 25.0 °C		
					Pressure = 759 mmHg		
Rota Meter Reading	Actual Flow Rate (l/min)				Deviation (l/min)	Permissible Deviation (l/min)	Status
	1	2	3	Average			
0.01	0.01	0.01	0.01	0.010	0.0000	±0.05	Pass
0.05	0.04	0.04	0.05	0.043	0.0058	±0.10	Pass
0.10	0.09	0.09	0.09	0.090	0.0000	±0.15	Pass
0.20	0.19	0.20	0.20	0.197	0.0058	±0.20	Pass

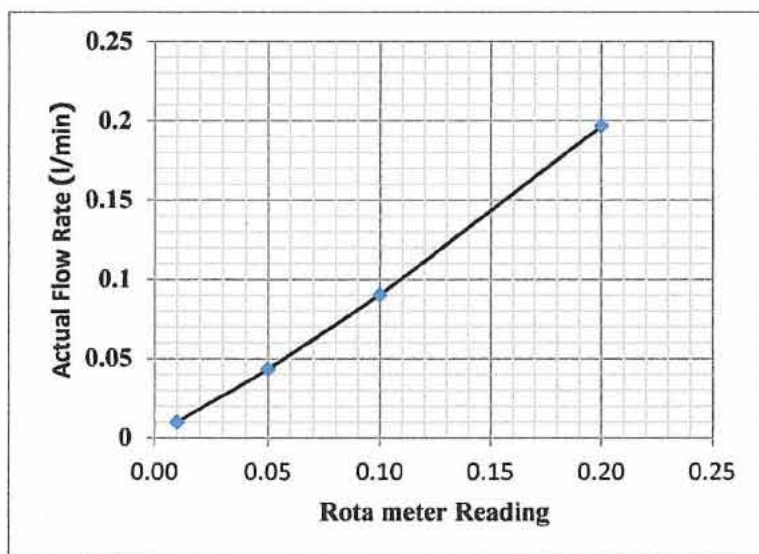

Calibrated by



Approved by



Industrial Hygiene Specialist

CALIBRATION TEST REPORT

Instrument : AIR CHECK SAMPLER (Low Flow)

Serial No. 038545

Model : 224-PC X R8


Manufacture : SKC (INC)

Date of Calibration : MARCH 11, 2024

AM-17

Next Time Calibration : MARCH 11, 2025


Standard Criteria : Rota Meter					Ambient Condition		
SKC Model1355EZ30 S/N 0107070345011/003					Temperature = 25.0 °C		
					Pressure = 759 mmHg		
Rota Meter Reading	Actual Flow Rate (l/min)				Deviation (l/min)	Permissible Deviation (l/min)	Status
	1	2	3	Average			
0.01	0.01	0.01	0.01	0.010	0.0000	±0.05	Pass
0.05	0.05	0.06	0.04	0.050	0.0100	±0.10	Pass
0.10	0.10	0.10	0.09	0.097	0.0058	±0.15	Pass
0.20	0.20	0.20	0.21	0.203	0.0058	±0.20	Pass

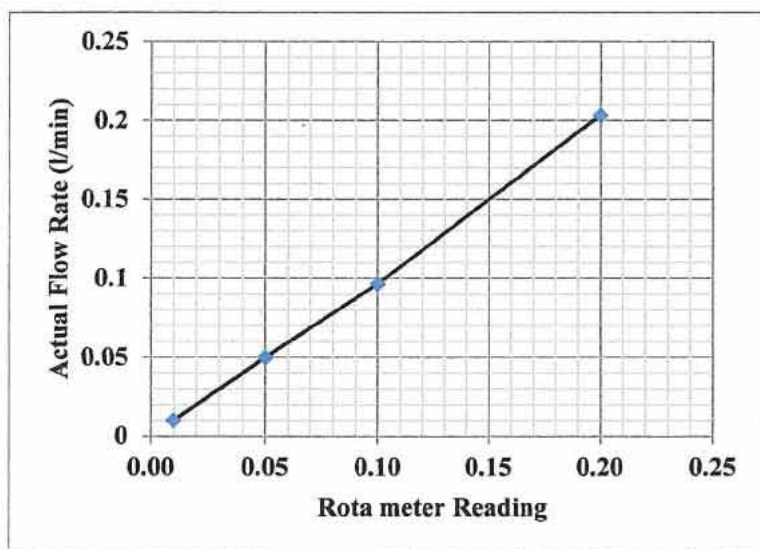

Calibrated by



Approved by

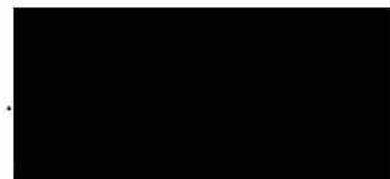

Industrial Hygiene Specialist

CALIBRATION TEST REPORT

Instrument : AIR CHECK SAMPLER (Low Flow)

Serial No. 038566

Model : 224-PC X R8


Manufacture : SKC (INC)

Date of Calibration : MARCH 11, 2024

AM-18

Next Time Calibration : MARCH 11, 2025

Standard Criteria : Rota Meter					Ambient Condition		
SKC Model1355EZ30 S/N 0107070345011/003					Temperature = 25.0 °C		
					Pressure = 759 mmHg		
Rota Meter Reading	Actual Flow Rate (l/min)				Deviation (l/min)	Permissible Deviation (l/min)	Status
	1	2	3	Average			
0.01	0.01	0.01	0.01	0.010	0.0000	±0.05	Pass
0.05	0.05	0.04	0.04	0.043	0.0058	±0.10	Pass
0.10	0.10	0.10	0.09	0.097	0.0058	±0.15	Pass
0.20	0.20	0.19	0.19	0.193	0.0058	±0.20	Pass

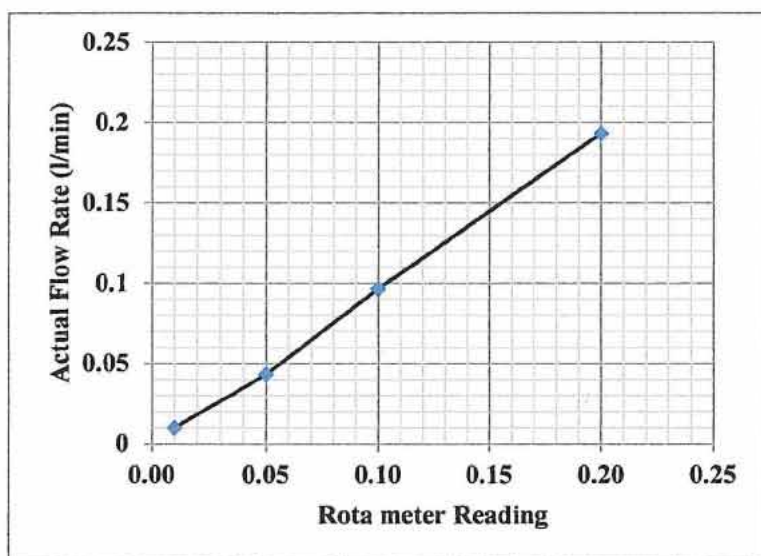

Calibrated by



Approved by



Industrial Hygiene Specialist

CALIBRATION TEST REPORT

Instrument : AIR CHECK SAMPLER (Low Flow)

Serial No. A122840

Model : 224-PC X R8


Manufacture : SKC (INC)

Date of Calibration : MARCH 11, 2024

AM-20

Next Time Calibration : MARCH 11, 2025


Standard Criteria : Rota Meter					Ambient Condition		
SKC Model1355EZ30 S/N 0107070345011/003					Temperature = 25.0 °C		
					Pressure = 759 mmHg		
Rota Meter Reading	Actual Flow Rate (l/min)				Deviation (l/min)	Permissible Deviation (l/min)	Status
	1	2	3	Average			
0.01	0.01	0.01	0.01	0.010	0.0000	±0.05	Pass
0.05	0.05	0.04	0.05	0.047	0.0058	±0.10	Pass
0.10	0.10	0.10	0.09	0.097	0.0058	±0.15	Pass
0.20	0.19	0.21	0.19	0.197	0.0115	±0.20	Pass

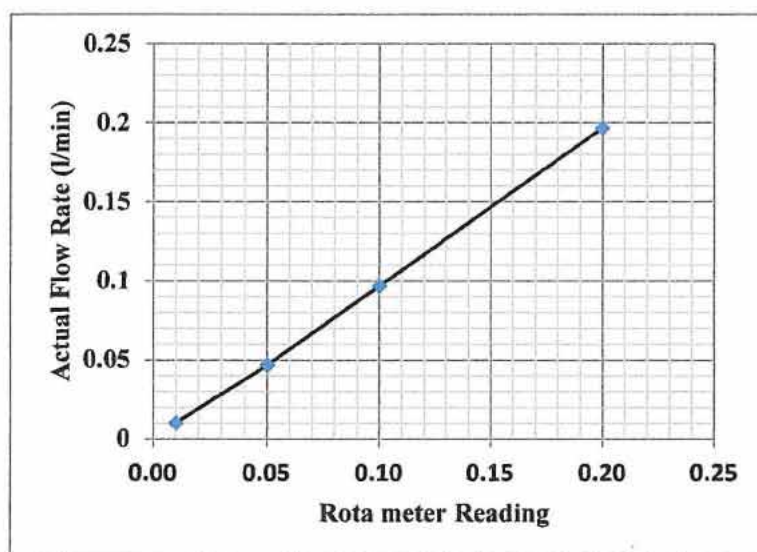

Calibrated by



Approved by

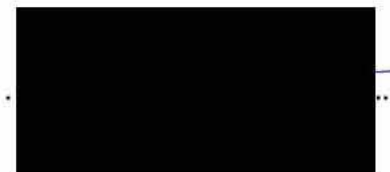

Industrial Hygiene Specialist

CALIBRATION TEST REPORT

Instrument : AIR CHECK SAMPLER (Low Flow)

Serial No. 20150601080

Model : BDX-II


Manufacture : Gilian

Date of Calibration : MARCH 11, 2024

GN-04

Next Time Calibration : MARCH 11, 2025

Standard Criteria : Rota Meter					Ambient Condition		
SKC Model1355EZ30 S/N 0107070345011/003					Temperature = 25.0 °C		
					Pressure = 759 mmHg		
Rota Meter Reading	Actual Flow Rate (l/min)				Deviation (l/min)	Permissible Deviation (l/min)	Status
	1	2	3	Average			
0.01	0.01	0.01	0.01	0.010	0.0000	±0.05	Pass
0.05	0.05	0.06	0.05	0.053	0.0058	±0.10	Pass
0.10	0.10	0.09	0.10	0.097	0.0058	±0.15	Pass
0.20	0.20	0.20	0.19	0.197	0.0058	±0.20	Pass

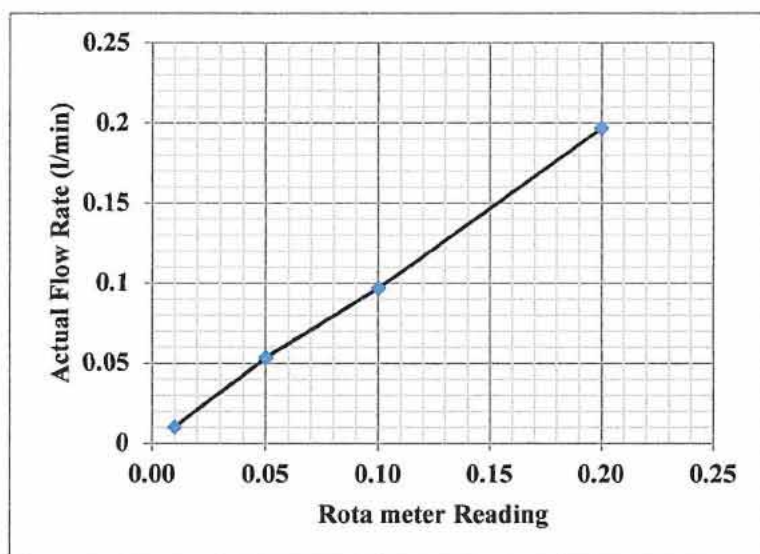

Calibrated by



Approved by



Industrial Hygiene Specialist

CALIBRATION TEST REPORT

Instrument : AIR CHECK SAMPLER (Low Flow)

Serial No. 20170104055

Model : BDX-II


Manufacture : Gilian

Date of Calibration : MARCH 11, 2024


GN-06

Next Time Calibration : MARCH 11, 2025

Standard Criteria : Rota Meter					Ambient Condition		
SKC Model1355EZ30 S/N 0107070345011/003					Temperature = 25.0 °C		
					Pressure = 759 mmHg		
Rota Meter Reading	Actual Flow Rate (l/min)				Deviation (l/min)	Permissible Deviation (l/min)	Status
	1	2	3	Average			
0.01	0.01	0.01	0.01	0.010	0.0000	±0.05	Pass
0.05	0.05	0.05	0.05	0.050	0.0000	±0.10	Pass
0.10	0.10	0.09	0.10	0.097	0.0058	±0.15	Pass
0.20	0.21	0.21	0.20	0.207	0.0058	±0.20	Pass

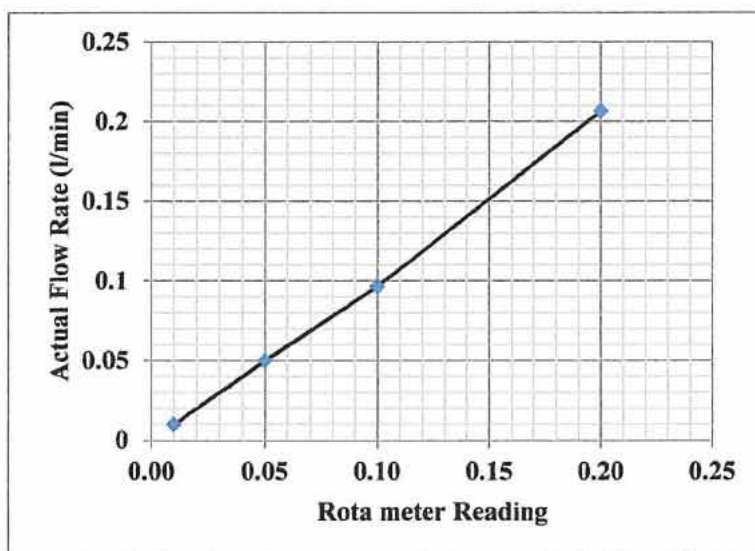

Calibrated by

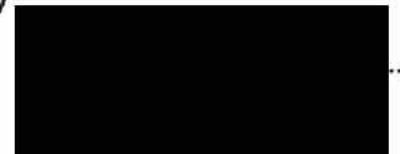

Approved by



Industrial Hygiene Specialist

CALIBRATION TEST REPORT

Instrument : AIR CHECK SAMPLER (Low Flow)

Serial No. 20170104061

Model : BDX-II


Manufacture : Gilian

Date of Calibration : MARCH 11, 2024

GN-07

Next Time Calibration : MARCH 11, 2025

Standard Criteria : Rota Meter					Ambient Condition		
SKC Model1355EZ30 S/N 0107070345011/003					Temperature = 25.0 °C		
					Pressure = 759 mmHg		
Rota Meter Reading	Actual Flow Rate (l/min)				Deviation (l/min)	Permissible Deviation (l/min)	Status
	1	2	3	Average			
0.01	0.01	0.01	0.01	0.010	0.0000	±0.05	Pass
0.05	0.04	0.05	0.05	0.047	0.0058	±0.10	Pass
0.10	0.10	0.09	0.10	0.097	0.0058	±0.15	Pass
0.20	0.20	0.20	0.21	0.203	0.0058	±0.20	Pass

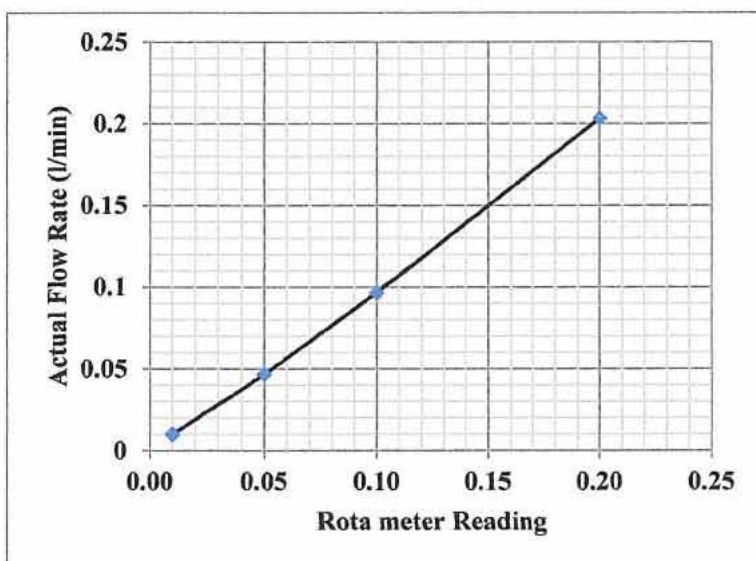

Calibrated by



Approved by



Industrial Hygiene Specialist

CALIBRATION TEST REPORT

Instrument : AIR CHECK SAMPLER (Low Flow)

Serial No. 20170104062

Model : BDX-II


Manufacture : Gilian

Date of Calibration : MARCH 11, 2024


GN-08

Next Time Calibration : MARCH 11, 2025


Standard Criteria : Rota Meter					Ambient Condition		
SKC Model1355EZ30 S/N 0107070345011/003					Temperature = 25.0 °C		
					Pressure = 759 mmHg		
Rota Meter Reading	Actual Flow Rate (l/min)				Deviation (l/min)	Permissible Deviation (l/min)	Status
	1	2	3	Average			
0.01	0.01	0.01	0.01	0.010	0.0000	±0.05	Pass
0.05	0.06	0.06	0.05	0.057	0.0058	±0.10	Pass
0.10	0.10	0.09	0.10	0.097	0.0058	±0.15	Pass
0.20	0.19	0.19	0.20	0.193	0.0058	±0.15	Pass

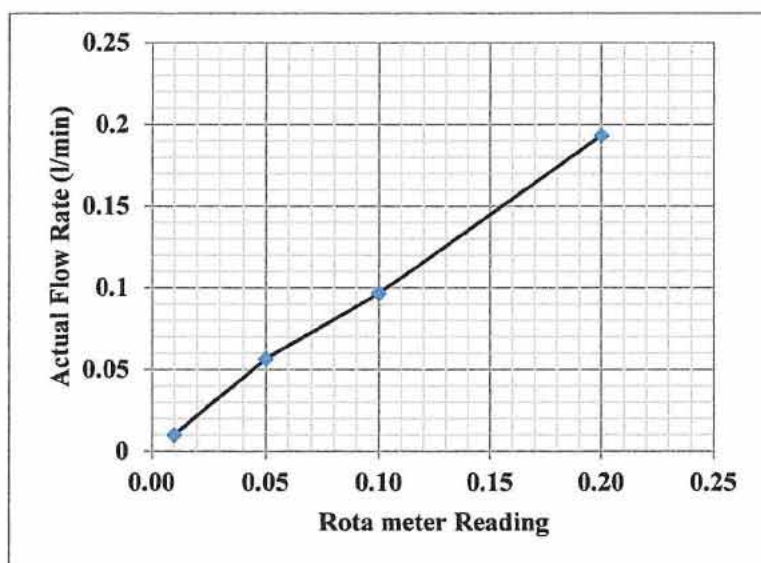

Calibrated by

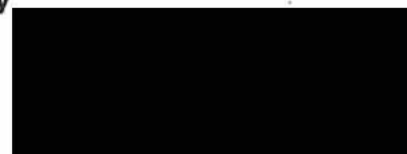

Approved by

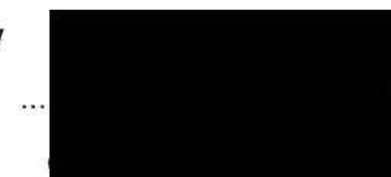

Industrial Hygiene Specialist

CALIBRATION TEST REPORT

Instrument : AIR CHECK SAMPLER (High Flow)

Serial No. 038536

Model : 224-PC X R8


Manufacture : SKC (INC)

Date of Calibration : MARCH 11, 2024

AM-15

Next Time Calibration : MARCH 11,2025


Standard Criteria : Rota Meter					Ambient Condition		
SKC Model1355EZ30 S/N 0107070345011/003					Temperature = 25.0 °C		
					Pressure = 759 mmHg		
Rota Meter Reading	Actual Flow Rate (l/min)				Deviation (l/min)	Permissible Deviation (l/min)	Status
	1	2	3	Average			
0.5	0.50	0.55	0.50	0.517	0.0289	±0.05	Pass
1.0	1.00	1.00	1.05	1.017	0.0289	±0.10	Pass
2.0	2.05	2.05	2.00	2.033	0.0289	±0.15	Pass
3.0	2.80	2.90	2.80	2.833	0.0577	±0.20	Pass

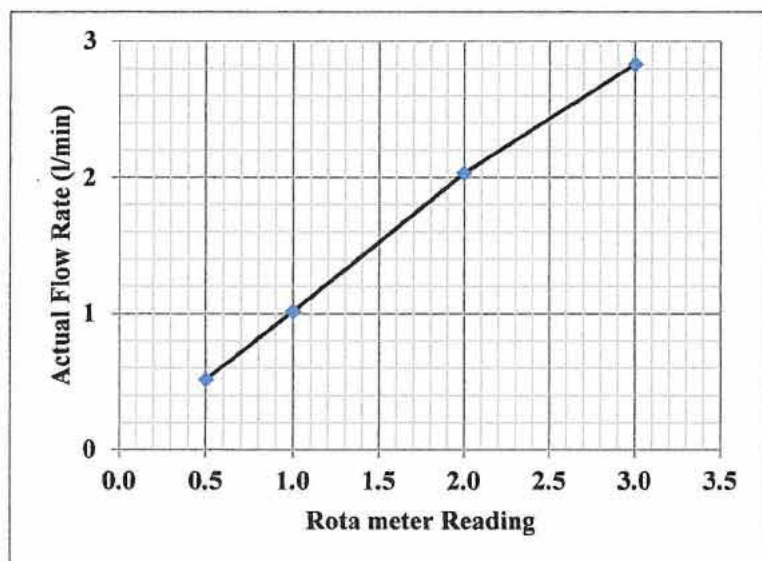

Calibrated by



Approved by

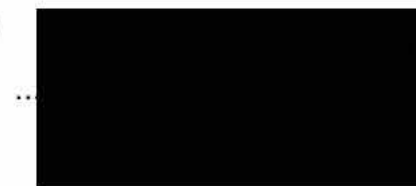

Industrial Hygiene Specialist

CALIBRATION TEST REPORT

Instrument : AIR CHECK SAMPLER (High Flow)

Serial No. 038556

Model : 224-PC X R8


Manufacture : SKC (INC)

Date of Calibration : MARCH 11,2024

AM-16

Next Time Calibration : MARCH 11,2025

Standard Criteria : Rota Meter SKC Model1355EZ30 S/N 0107070345011/003					Ambient Condition Temperature = 25.0 °C Pressure = 759 mmHg		
Rota Meter Reading	Actual Flow Rate (l/min)				Deviation (l/min)	Permissible Deviation (l/min)	Status
	1	2	3	Average			
0.5	0.55	0.55	0.60	0.567	0.0289	±0.05	Pass
1.0	1.05	1.05	1.10	1.067	0.0289	±0.10	Pass
2.0	1.95	1.95	1.90	1.933	0.0289	±0.15	Pass
3.0	2.80	2.85	2.90	2.850	0.0500	±0.20	Pass

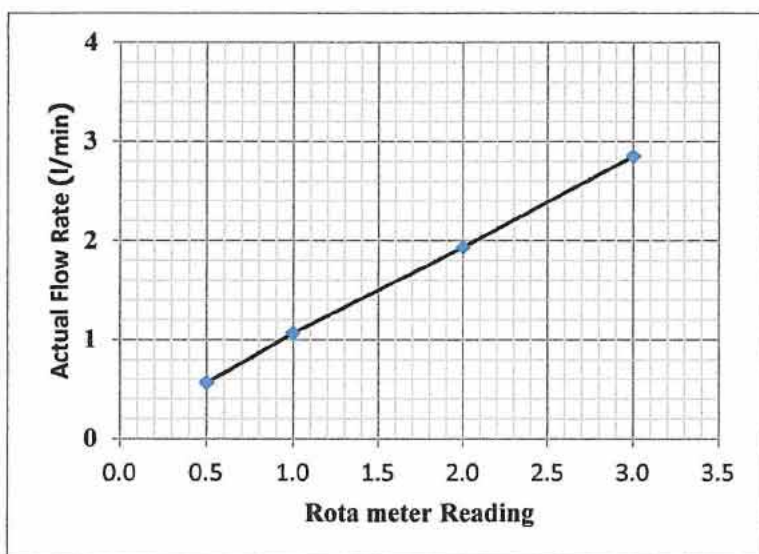

Calibrated by



Approved by



Industrial Hygiene Specialist

CALIBRATION TEST REPORT

Instrument : AIR CHECK SAMPLER (High Flow)

Serial No. 038545

Model : 224-PC X R8


Manufacture : SKC (INC)

Date of Calibration : MARCH 11, 2024

AM-17

Next Time Calibration : MARCH 11,2025

Standard Criteria : Rota Meter					Ambient Condition		
SKC Model1355EZ30 S/N 0107070345011/003					Temperature = 25.0 °C		
					Pressure = 759 mmHg		
Rota Meter Reading	Actual Flow Rate (l/min)				Deviation (l/min)	Permissible Deviation (l/min)	Status
	1	2	3	Average			
0.5	0.55	0.60	0.55	0.567	0.0289	±0.05	Pass
1.0	1.00	1.05	1.05	1.033	0.0289	±0.10	Pass
2.0	1.95	1.90	1.90	1.917	0.0289	±0.15	Pass
3.0	2.95	2.80	2.85	2.867	0.0764	±0.20	Pass

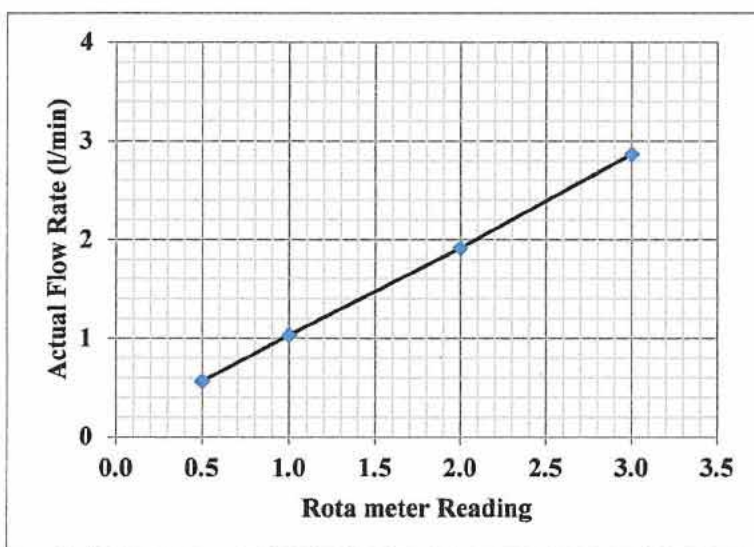

Calibrated by



Approved by



Industrial Hygiene Specialist

CALIBRATION TEST REPORT

Instrument : AIR CHECK SAMPLER (High Flow)

Serial No. 038566

Model : 224-PC X R8


Manufacture : SKC (INC)

Date of Calibration : MARCH 11, 2024

AM-18

Next Time Calibration : MARCH 11,2025

Standard Criteria : Rota Meter					Ambient Condition		
SKC Model1355EZ30 S/N 0107070345011/003					Temperature = 25.0 °C		
					Pressure = 759 mmHg		
Rota Meter Reading	Actual Flow Rate (l/min)				Deviation (l/min)	Permissible Deviation (l/min)	Status
	1	2	3	Average			
0.5	0.55	0.45	0.45	0.483	0.0577	±0.05	Pass
1.0	0.95	1.00	1.05	1.000	0.0500	±0.10	Pass
2.0	1.95	1.85	1.85	1.883	0.0577	±0.15	Pass
3.0	2.85	2.85	3.00	2.900	0.0866	±0.20	Pass

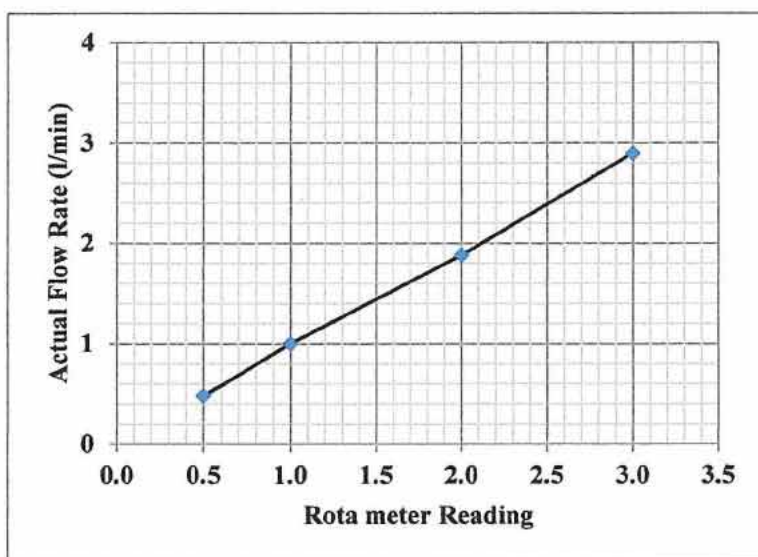

Calibrated by



Approved by



Industrial Hygiene Specialist

CALIBRATION TEST REPORT

Instrument : AIR CHECK SAMPLER (High Flow)

Serial No. A122840

Model : 224-PC X R8


Manufacture : SKC (INC)

Date of Calibration : MARCH 11, 2024

AM-20

Next Time Calibration : MARCH 11,2025

Standard Criteria : Rota Meter					Ambient Condition		
SKC Model1355EZ30 S/N 0107070345011/003					Temperature = 25.0 °C		
					Pressure = 759 mmHg		
Rota Meter Reading	Actual Flow Rate (l/min)				Deviation (l/min)	Permissible Deviation (l/min)	Status
	1	2	3	Average			
0.5	0.50	0.50	0.45	0.483	0.0289	±0.05	Pass
1.0	1.10	1.05	1.00	1.050	0.0500	±0.10	Pass
2.0	2.00	1.95	2.05	2.000	0.0500	±0.15	Pass
3.0	2.90	2.85	2.95	2.966	0.0500	±0.20	Pass

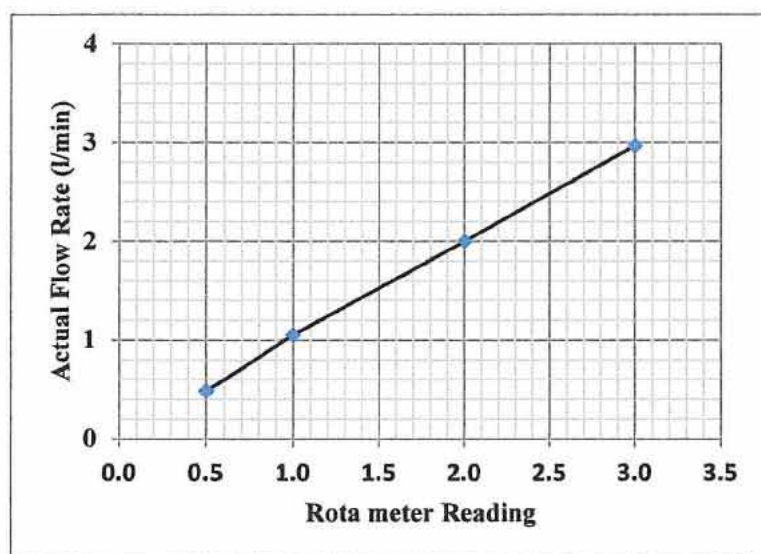

Calibrated by



Approved by



Industrial Hygiene Specialist

CALIBRATION TEST REPORT

Instrument : AIR CHECK SAMPLER (High Flow)

Serial No. 20150601080

Model : BDX-II


Manufacture : Gilian

Date of Calibration : MARCH 11, 2024

GN-04

Next Time Calibration : MARCH 11,2025

Standard Criteria : Rota Meter SKC Model1355EZ30 S/N 0107070345011/003					Ambient Condition Temperature = 25.0 °C Pressure = 759 mmHg		
Rota Meter Reading	Actual Flow Rate (l/min)				Deviation (l/min)	Permissible Deviation (l/min)	Status
	1	2	3	Average			
0.5	0.55	0.55	0.50	0.533	0.0289	±0.05	Pass
1.0	1.10	1.10	1.15	1.117	0.0289	±0.10	Pass
2.0	2.00	2.05	2.05	2.033	0.0289	±0.15	Pass
3.0	3.00	3.00	2.95	2.983	0.0289	±0.20	Pass

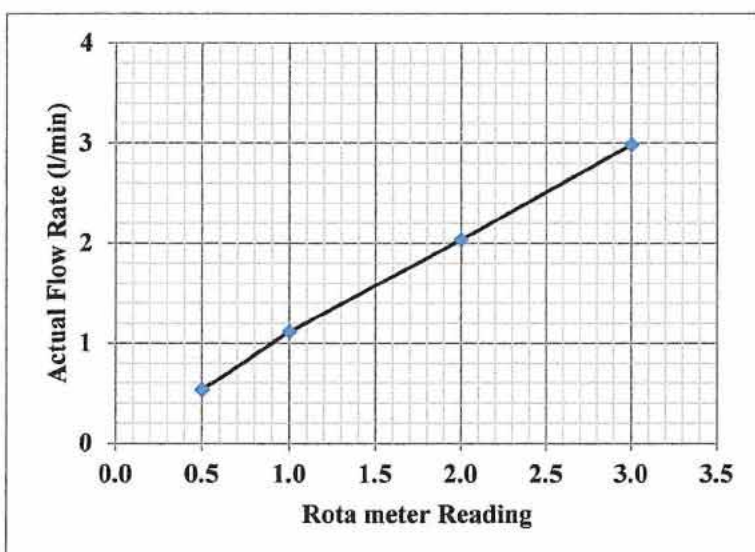

Calibrated by



Approved by



Industrial Hygiene Specialist

CALIBRATION TEST REPORT

Instrument : AIR CHECK SAMPLER (High Flow)

Serial No. 20170104055

Model : BDX-II


Manufacture : Gilian

Date of Calibration : MARCH 11, 2024

GN-06

Next Time Calibration : MARCH 11, 2025

Standard Criteria : Rota Meter					Ambient Condition		
SKC Model1355EZ30 S/N 0107070345011/003					Temperature = 25.0 °C		
					Pressure = 759 mmHg		
Rota Meter Reading	Actual Flow Rate (l/min)				Deviation (l/min)	Permissible Deviation (l/min)	Status
	1	2	3	Average			
0.5	0.45	0.45	0.50	0.467	0.0289	±0.05	Pass
1.0	1.05	1.05	1.00	1.033	0.0289	±0.10	Pass
2.0	2.00	2.05	2.10	2.050	0.0500	±0.15	Pass
3.0	2.85	2.95	2.80	2.867	0.0764	±0.20	Pass

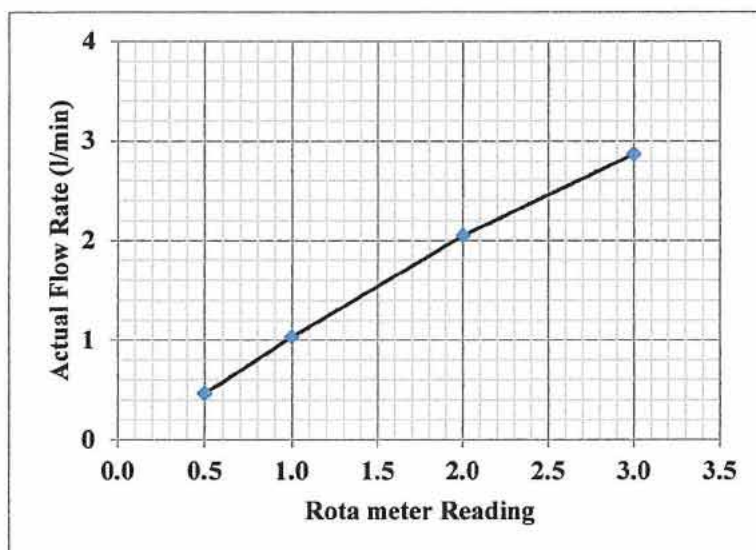

Calibrated by

[Redacted Signature]

Approved by

[Redacted Signature]

Industrial Hygiene Specialist

CALIBRATION TEST REPORT

Instrument : AIR CHECK SAMPLER (High Flow)

Serial No. 20170104061

Model : BDX-II


Manufacture : Gilian

Date of Calibration : MARCH 11, 2024

GN-07

Next Time Calibration : MARCH 11,2025


Standard Criteria : Rota Meter					Ambient Condition		
SKC Model1355EZ30 S/N 0107070345011/003					Temperature = 25.0 °C		
					Pressure = 759 mmHg		
Rota Meter Reading	Actual Flow Rate (l/min)				Deviation (l/min)	Permissible Deviation (l/min)	Status
	1	2	3	Average			
0.5	0.45	0.50	0.45	0.467	0.0289	±0.05	Pass
1.0	1.05	1.00	1.05	1.033	0.0289	±0.10	Pass
2.0	2.10	2.10	2.00	2.067	0.0577	±0.15	Pass
3.0	3.00	2.95	2.95	2.967	0.0289	±0.20	Pass

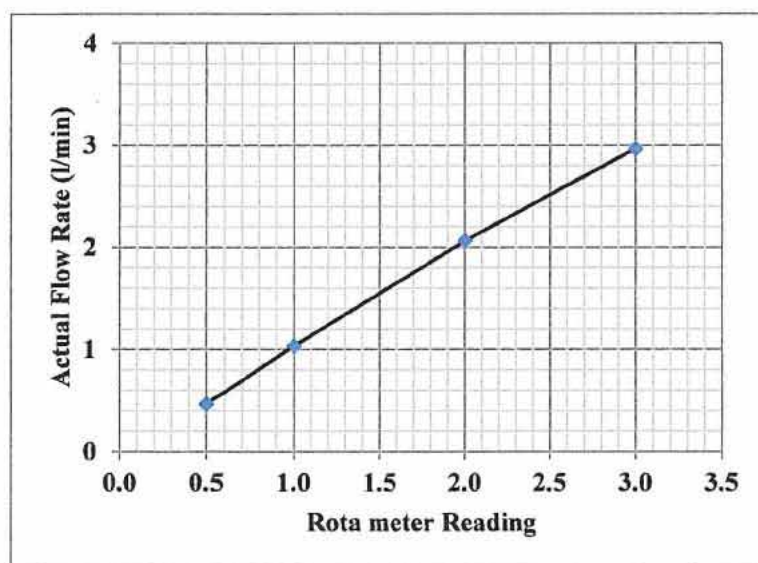

Calibrated by



Approved by

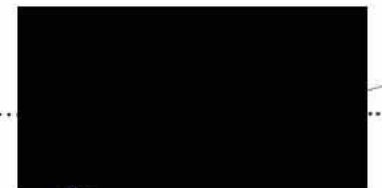

Industrial Hygiene Specialist

CALIBRATION TEST REPORT

Instrument : AIR CHECK SAMPLER (High Flow)

Serial No. 20170104062

Model : BDX-II


Manufacture : Gillan

Date of Calibration : MARCH 11, 2024


GN-08

Next Time Calibration : MARCH 11,2025

Standard Criteria : Rota Meter					Ambient Condition		
SKC Model1355EZ30 S/N 0107070345011/003					Temperature = 25.0 °C		
					Pressure = 759 mmHg		
Rota Meter Reading	Actual Flow Rate (l/min)				Deviation (l/min)	Permissible Deviation (l/min)	Status
	1	2	3	Average			
0.5	0.50	0.50	0.45	0.483	0.0289	±0.05	Pass
1.0	1.00	1.00	1.05	1.017	0.0289	±0.10	Pass
2.0	2.00	1.95	1.90	1.950	0.0500	±0.15	Pass
3.0	2.95	2.90	2.85	2.900	0.0500	±0.15	Pass

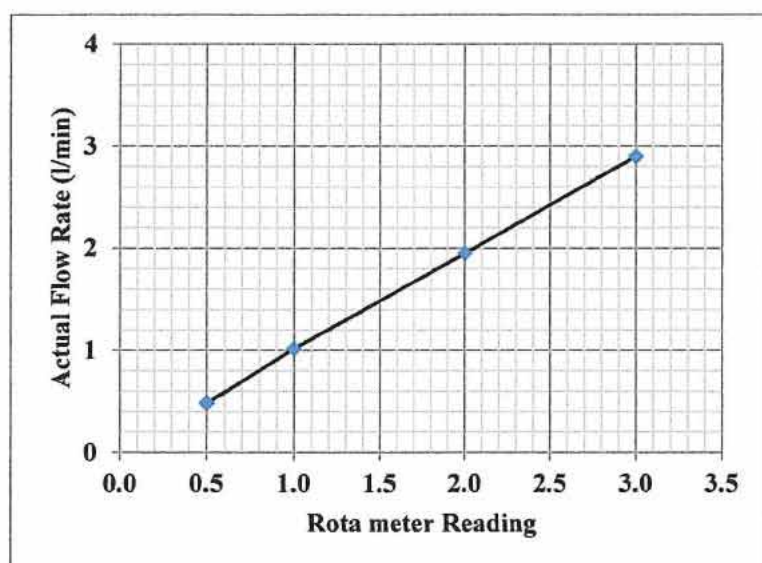

Calibrated by

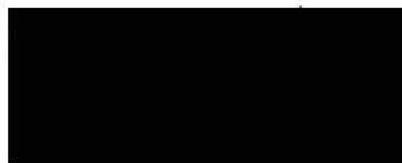

Approved by



Industrial Hygiene Specialist



ID LINE : IEC17025

69/29 Moo 1 Klongsi Klongluang Pathumthani 12120 (Thailand) Tel: (662) 193-2220 5 ศัสาย www.สอเนเทียมและเครื่องวัด.คอม



Certificate of Calibration


Certificate Number : SPR24030129-1 Page : 1 of 3

Customer : Life and Environment Co., Ltd.
90, 92, 94 Soi On-Nuch 64, Srinakarin Rd., On-Nuch, Suanluang,
Bangkok 10250


Equipment Name	: Rota Flow Meter		
Manufacturer	: Brooks Instrument Division		
Model	: 1355EZ30		
Serial Number	: 0107070345011/003		
ID. Number	: ROTA CAL.02		
Environmental Conditions			
Ambient Temperature	: 23 °C ± 2 °C	Received Date	: 09 Mar 2024
Relative Humidity	: 50 % ± 15 %	Calibration Date	: 09 Mar 2024
Location of Calibration	: In-Lab	Recommend Due Date	: 09 Mar 2025
Calibration Procedure	: SP-CPM-04-13	Date of Issue	: 10 Mar 2024

Method of Calibration

This certifies that the above instrument was calibrated in compliance with the calibration system requirement of ISO/IEC 17025:2017 in accordance with reference procedure. Standards used to perform this calibration are certified by to NIST or equivalent, National metrology institute, Natural physical constants, consensus standards. The result reported herein apply only to the calibration of the item described above as received. Our decision rule is to contact the customer if the item pass and fail calibration when the results include the uncertainties and the customer must determine if the results meets their needs. The calibration certificate shall not be reproduced except in full, without written approval of SP Metrology System (Thailand).

Calibrated by : 
Calibration Officer

Approved by : 
Authorized Signatory



Page : 2 of 3

SP-FM-04-15 rev.0



ID LINE : IEC17025



Result of Calibration

Certificate No. : SPR24030129-1

Page : 3 of 3

Range : 0 to 5 L/Min

Function : Air Flow Measurement

Unit : L/Min

Calibration Point	UUC Reading	Standard Reading	UUC Error	K Factor Value	Uncertainty (±)
0.02	0.02	0.03432	-0.01432	1.716000	0.058
0.10	0.1	0.04881	0.05119	0.488100	0.058
1.00	1.0	0.9723	0.0277	0.972300	0.059
2.00	2.0	2.0044	-0.0044	1.002200	0.061
3.00	3.0	3.0270	-0.0270	1.009000	0.065

Note:

The result of calibration was found accurate as show on date and place of calibration only.
This Certificate is not certified for any commercial transaction.

Measurement Uncertainty

The reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor $k = 2$, providing a level of confidence approximately 95 %

- End of Certificate -



บริษัท พาราไซแอนติฟิค จำกัด
BARA SCIENTIFIC CO., LTD.

PREVENTIVE MAINTENANCE/ CALIBRATION

GC SYSTEM

GC-14B/C-R5A

ID NO.	:
REPORT NO.	:C-A3-TK-6611-0300
DATE OF REPORT	:15 November 2023
COMPLETION DATE	:15 November 2023
NEXT DUE DATE	:On November 2024

GAS CHROMATOGRAPHY

SERIAL NUMBER	C10733000756SA
CUSTOMER	LIFE AND ENVIRONMENT CO., LTD.
ADDRESS	90,92,94 SOI ON-NUCH 64, SRINAKARIN ROAD, ON-NUCH SUANLUANG, BANGKOK 10250.
ATTENTION	KHUN TUNYALUCK KREEPANICH
PHONE	02-320-0277-8 EXT.304,308
FAX	023200293
DONE BY	Mr.Thanawat Pumpaka
SERVICE REPORT NO.	TK-6611-0300

SIGNED FOR AND ON BEHALF OF
BARA SCIENTIFIC CO.,LTD.





บริษัท พาราไซแอนติฟิค จำกัด
BARA SCIENTIFIC CO., LTD.

CERTIFICATE

THIS CERTIFIES THE PERFORMANCE OF SHIMADZU GAS CHROMATOGRAPHY AT

LIFE AND ENVIROMENT CO., LTD.ADDRESS : 90,92,94 SOI ON-NUCH 64,
SRINAKARIN ROAD,SUANLUANG, BANGKOK 10250.

SYSTEM CONFIGURATION : GC-14B, C-R5A

DETECTOR TYPE : FLAME IONIZATION DETECTOR (FID)

METHOD : SENSITIVITY TEST OF FID BY SHIMADZU CORPORATION, JAPAN.

CHEMICAL : N-HEXADECANE(C₁₆) 100ng/uL (HEPTANE SOVENT)

SPECIFICATION OF FID :S(C/g)OF C16 IS MORE THAN 0.01(C/g)

RESULT : SENSITIVITY OF FID CH1 = 0.0163 C/g

REPRODUCIBILITY : Area Value CH1 CV \leq 10.00 % = 1.566 %

Retention Time CH1 CV \leq 2.00 % = 0.348 %

ISSUED ON : 15 November 2023

ISSUED AT : SERVICE SECTION, BARASCIENTIFIC CO.,LTD.

APPROVED BY :



SERVICE ENGINEER



**PREVENTIVE MAINTENANCE/
CALIBRATION**

GC SYSTEM


GC-14B/C-R5A

ID NO.	: -
REPORT NO.	: C-A3-TK-6711-0257
DATE OF REPORT	: 13 November 2024
COMPLETION DATE	: 13 November 2024
NEXT DUE DATE	: ON November 2025

GAS CHROMATOGRAPHY

SERIAL NUMBER	C10733000756SA
CUSTOMER	LIFE AND ENVIRONMENT CO., LTD.
ADDRESS	90,92,94 SOI ON-NUCH 64, SRINAKARIN ROAD, ON-NUCH SUANLUANG, BANGKOK 10250.
ATTENTION	KHUN TUNYALUCK KREEPANICH
PHONE	02-320-0277-8 EXT.304,308
FAX	023200293
DONE BY	Mr.Nattapon Ngamsang
SERVICE REPORT NO.	C-A3-TK-6711-0257

SIGNED FOR AND ON BEHALF OF
BARA SCIENTIFIC CO., LTD.

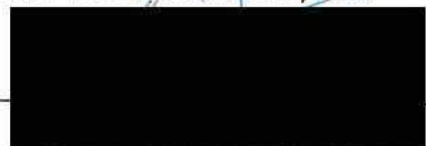

อนุมัติใช้วันที่ 3 มีนาคม 2553



บริษัท พาราไซแอนติฟิค จำกัด
BARA SCIENTIFIC CO., LTD.

CERTIFICATE

THIS CERTIFIES THE PERFORMANCE OF SHIMADZU GAS CHROMATOGRAPHY AT

LIFE AND ENVIROMENT CO., LTD.ADDRESS : 90,92,94 SOI ON-NUCH 64,
SRINAKARIN ROAD,SUANLUANG, BANGKOK 10250.

SYSTEM CONFIGURATION : GC-14B, C-R5A

DETECTOR TYPE : FLAME IONIZATION DETECTOR (FID)

METHOD : SENSITIVITY TEST OF FID BY SHIMADZU CORPORATION, JAPAN.

CHEMICAL : N-HEXADECANE(C₁₆) 100ng/uL (HEPTANE SOVENT)

SPECIFICATION OF FID :S(C/g)OF C16 IS MORE THAN 0.01(C/g)

RESULT : SENSITIVITY OF FID CH1 = 0.0115 C/g


REPRODUCIBILITY : Area Value CH1 CV \leq 10.00 % = 3.079 %

Retention Time CH1 CV \leq 2.00 % = 0.363 %

ISSUED ON : 13 November 2024

ISSUED AT : SERVICE SECTION, BARASCIENTIFIC CO.,LTD.

APPROVED BY :



SERVICE ENGINEER



Certificate of Calibration

Equipment:	SPECTROPHOTOMETER	Certificate No.:	C06230594
Model:	CE 1011	Issued Date:	14 December 2023
Serial No. (or ID.):	920-252	Job No.:	WO-00011851
Manufacturer:	CECIL	Page:	1 of 2
Condition:	In Condition		

Customer: LIFE & ENVIRONMENT CO., LTD.
90, 92, 94 Soi On-nuch 64, Srinakarin Road,
On-nuch, Suanluang, Bangkok 10250 Thailand.

Environment Condition:

Temperature	24.7	°C	±	0.2	°C
Humidity	58.7	%RH	±	0.5	%RH

Calibration Place: LIFE & ENVIRONMENT CO., LTD. (Air Testing Laboratory)
90, 92, 94 Soi On-nuch 64, Srinakarin Road,
On-nuch, Suanluang, Bangkok 10250 Thailand.

Calibration By: Miss.Kaewkan Suradech

Calibration Date: 13 December 2023

The Method used: In house method, CAL-WI-24, base on ASTM E 275-08 and ASTM E 387-04


Traceability: This certificate is traceable to the CRM maintained by National Institute of Standards and Technology (NIST) through Starna Scientific Limited.

The standard for Wavelength Certificate No. 105931 and 105898

The standard for Photometric Certificate No. 105940



Person in charge

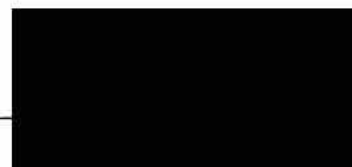

Authorized signatory

This certificate is issued the units of measurement according to the International System of Units (SI). It provides traceability of measurement to international or national standard or other recognized national standard laboratories.

The measurement uncertainty stated is the expanded uncertainty which is obtained from the standard uncertainty multiplied by the coverage factor ($k=2$) to provide a level of confidence of approximately 95%. It is determined in accordance with the Guide to Expression of Uncertainty in Measurement (GUM).

These results may be affected by deviations from specified conditions. The results relate only to the items tested, calibrated or sampled. The report shall not be reproduced except in full without approval of DKSH Technology Limited.

บริษัท ดีเคเอสเอช เทคโนโลยี จำกัด
DKSH Technology Limited

2533 ถนนสุขุมวิท แขวงบางจาก เขตพระโขนง กรุงเทพมหานคร 10260
2533 Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260

Phone: +66 2639 7000 Email: info.calibration@dksh.com Website: www.dksh.com/scientific-thailand

Calibration Results:
Without Adjustment
Wavelength Accuracy (nm), The spectral bandwidth of Std at 5 nm and UUC at 8 nm

Standard Wavelength	Unit Under Calibration	Correction	Uncertainty
418.40	421.0	-2.60	0.13
447.20	450.3	-3.10	0.13
459.30	459.5	-0.20	0.13
537.00	539.2	-2.20	0.13
638.00	641.1	-3.10	0.13
585.56	589.5	-3.94	0.13

Photometric Accuracy (Absorbance)

Wavelength	Standard absorbance	Unit Under Calibration	Correction	Uncertainty
420 nm	0.0000	0.000	0.0000	0.0045
	0.5890	0.590	-0.0010	0.0045
	0.7604	0.761	-0.0006	0.0045
	1.0241	1.032	-0.0079	0.0045
440 nm	0.0000	0.000	0.0000	0.0045
	0.5782	0.574	0.0042	0.0045
	0.7430	0.738	0.0050	0.0045
	1.0016	1.000	0.0016	0.0045
465 nm	0.0000	0.000	0.0000	0.0045
	0.5283	0.529	-0.0007	0.0045
	0.6854	0.686	-0.0006	0.0045
	0.9509	0.951	-0.0001	0.0045
546.1 nm	0.0000	0.000	0.0000	0.0045
	0.5457	0.544	0.0017	0.0045
	0.6944	0.693	0.0014	0.0045
	0.9965	0.996	0.0005	0.0045
590 nm	0.0000	0.000	0.0000	0.0045
	0.5837	0.578	0.0057	0.0045
	0.7223	0.715	0.0073	0.0045
	1.0935	1.084	0.0095	0.0045
635 nm	0.0000	0.000	0.0000	0.0045
	0.5675	0.564	0.0035	0.0045
	0.6900	0.685	0.0050	0.0045
	1.0862	1.080	0.0062	0.0045

The End of Certificate



Certificate of Calibration

Equipment:	Balance	Certificate No.:	C01241067
Model:	LA130S-F	Issued Date:	22 March 2024
Serial No. (or ID.):	16908811 (EP-AB-01/47)	Job No.:	WO-00021722
Manufacturer:	Sartorius	Page:	1 of 2
Condition:	In condition		

Customer: LIFE & ENVIRONMENT CO., LTD.
90, 92, 94 Soi On-nuch 64, Srinakarin Road, On-nuch,
Suanluang, Bangkok 10250 Thailand

Environment Condition: Temperature 26 °C ± 0.5 °C
Humidity 47 %RH ± 4.2 %RH


Calibration Place: LIFE & ENVIRONMENT CO., LTD. (Air (TSP/PM10) Testing Laboratory)
90, 92, 94 Soi On-nuch 64, Srinakarin Road, On-nuch,
Suanluang, Bangkok 10250 Thailand

Calibration By: Mr. Polawad Ruamlrup


Calibration Date: 22 March 2024

The Method used: In-house method, CAL-WI-47, based on UKAS Lab 14

Traceability: This certificate is traceable to the SI Units maintained by National Institute of Metrology (NIMT), Thailand through DKSH Technology Co., Ltd. Certificate No. C02240400



Person in charge

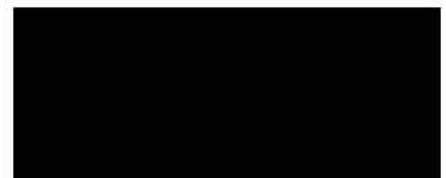

Authorized signatory

This certificate is issued the units of measurement according to the International System of Units (SI). It provides traceability of measurement to international or national standard or other recognized national standard laboratories.

The measurement uncertainty stated is the expanded uncertainty which is obtained from the standard uncertainty multiplied by the coverage factor ($k=2$) to provide a level of confidence of approximately 95%. It is determined in accordance with the Guide to Expression of Uncertainty in Measurement (GUM).

These results may be affected by deviations from specified conditions. The results relate only to the items tested, calibrated or sampled. The report shall not be reproduced except in full without approval of DKSH Technology Limited.

บริษัท ดีเคเอสเอช เทคโนโลยี จำกัด

DKSH Technology Limited

2533 ถนนสุขุมวิท แขวงบางจาก เขตพระโขนง กรุงเทพมหานคร 10260


2533 Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260

Phone: +66 2639 7000 Email: info.calibration@dksh.com Website: www.dksh.com/scientific-thailand

Calibration Results:

Without Adjustment

Eccentric Error: Weight to be 1/3 or 1/2 of Maximum capacity, taken from the center of the pan as a zero reference.

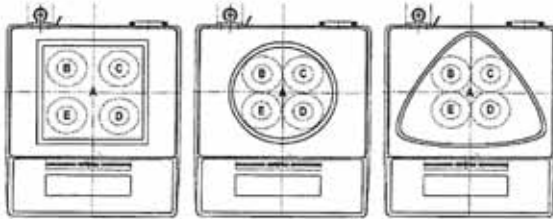

Nominal Test Value 5 (g)

Reference Points (g)				
A	B	C	D	E
-	0.0000	0.0001	0.0000	-0.0001

Repeatability: Determination of the standard deviation of weighing balance., Readability 0.0001 (g)

Nominal test value (g)	Standard Deviation
1	0.00005
10	0.00009

Error of indication from nominal or conventional mass value., Readability 0.0001 (g)

Nominal Value (g)	Conventional Mass (g)	Displayed Value (g)	Error of indication (g)	Uncertainty (g)	k
1	1.00001	1.0000	0.0000	0.00014	2.11
2	2.00002	2.0000	0.0000	0.00014	2.11
3	3.00003	2.9999	-0.0001	0.00015	2.11
4	4.00003	4.0000	0.0000	0.00015	2.10
5	5.00002	5.0001	0.0001	0.00014	2.11
6	6.00003	6.0000	0.0000	0.00015	2.10
7	7.00004	6.9999	-0.0001	0.00015	2.10
8	8.00005	8.0000	0.0000	0.00015	2.08
9	9.00005	9.0000	0.0000	0.00015	2.08
10	10.00001	10.0001	0.0001	0.00015	2.11


The End of Certificate

TEST REPORT

CUSTOMER NAME : All-Quip Co., Ltd. [บริษัท ออล ควิป จำกัด (สำนักงานใหญ่)]			
EQUIPMENT NAME : SO ₂ Analyzer			
MANUFACTURER : HORIBA	MODEL : APSA-370	SERIAL NO : 4AXYPEYX	
STANDARD GAS CONCENTRATION (PPM) : 53.29 PPM		CYLINDER NO : CC734373	
CYLINDER PRESSURE (PSI) : 1,400 PSI		CERTIFIED DATE : 12/05/2020	
CERTIFIED BY : AIRGAS		EXPIRED DATE : 12/05/2028	

TEST RESULTS

POINT NO	TEST RESULTS			
	IDEAL	ACTUAL	ERROR	%ERROR
ZERO	0.00	0.10	0.10	-
1	100.00	99.40	-0.6	-0.60
2	200.00	200.00	0.0	0.00
3	300.00	299.50	-0.5	-0.17
4	400.00	399.70	-0.3	-0.08
AVERAGE (%)				0.21

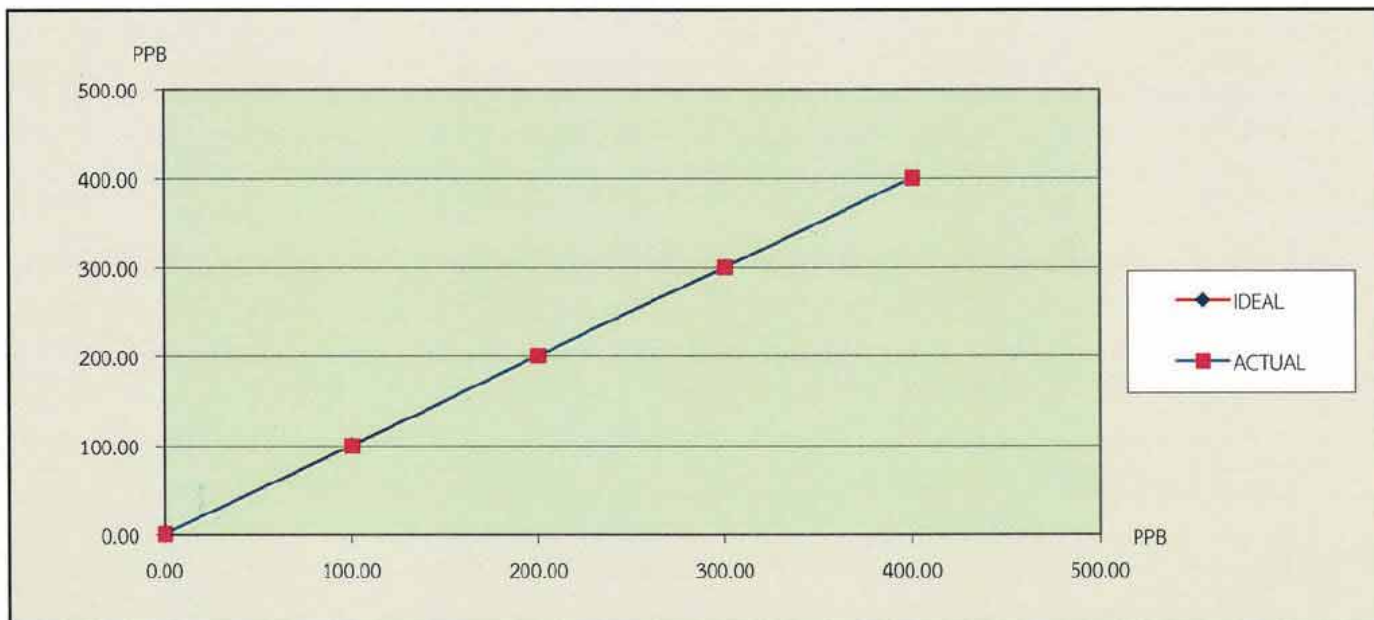

CALIBRATED BY : [REDACTED]

DATE : 15/2/24

CHECKED BY : [REDACTED]

DATE : 15/2/24



ต้องการข้อมูลทางด้านเทคนิคเพิ่มเติม : เจ้าหน้าที่ฝ่ายบริการหลังการขาย , โทร 02-868-0812 # 15-16 , E-Mail : Engineer@jiranatee.com

เลขที่ 63/14-15,67/35-36 ถนน ซอยเพชรเกษม 7/7/1 เพชรเกษม แขวงวัดท่าพระ เขตบางกอกใหญ่ กรุงเทพฯ 10600 โทร 02-868-0812-13 โทรสาร 02-868-1889

CHECK LIST

CUSTOMER NAME : All-Quip Co., Ltd. [บริษัท ออล คิวป์ จำกัด (สำนักงานใหญ่)]		
EQUIPMENT NAME : SO ₂ Analyzer		
MANUFACTURER : HORIBA	MODEL : APSA-370	SERIAL NO. : 4AXYPEYX

TEST VALUES				
NO.	Ambient SO ₂ Monitor	UNIT	BEFORE	AFTER
1	SIGNAL	mV (Voltage of the measured SO ₂ Value)	19.10	4.20
2	LAMP	mV (200mV to 1200 mV)	297.30	297.30
3	CELL	°C (Ambient tembient temperature +(5°C to 15°C))	34.00	34.00
4	PUMP	kPa (65 kPa or less)	43.60	43.60
5	AMBIENT	kPa	101.40	101.40
6	SAMPLE	L/min (0.6 L/min to 1.0 L/min)	-	-
7	DC 24 V	V (24 V ± 0.5 V)	23.90	23.90
8	DC 5 V	V (5 V ± 0.5 V)	4.90	4.90
9	SAMPLE SO2 Reading	PPB	3.80	0.80
10	Zero	PPB	3.10	0.10
11	Span	PPB	258.70	399.70

Remark : Reference EX-EN-019-56 , Ambient SO2 Monitor APSA-370 Operetion Manual Page #78

(Ambeint temperature = 5°C to 40°C)

อาการที่ตรวจพบ

รายละเอียดการดำเนินการ

- ทำ Calibration Zero/Span , Multipoint , เช็ค Dianostics

ผลการดำเนินการ

- เรียบร้อย เครื่องสามารถดำเนินการตรวจวัดได้ตามปกติ

CALIBRATED BY :

CHECKED BY :



DATE : 15/2/24

DATE : 15/2/24

ต้องการข้อมูลทางด้านเทคนิคเพิ่มเติม : เจ้าหน้าที่ฝ่ายบริการหลังการขาย , โทร 02-868-0812 # 15-16 , E-Mail : Engineer@jiranatee.com

เลขที่ 63/14-15 , 67/35-36 ซอยเพชรเกษม 7,7/1 ถนนเพชรเกษม แขวงวัดท่าพระ เขตบางกอกใหญ่ กรุงเทพฯ 10600 โทร : 02-868-0812-13 โทรสาร : 02-868-1889

Test Report Calibration

Ecotech EC9850 Sulphur Dioxide Analyzer

Issued By	Sithiporn Associates Company Limited	Calibration Date	22-Jan-2024
Owner Name	Life & Environment Co.,Ltd.	Product Brand	Ecotech
Certificate Number	34303	Type Systematic	Analyzer Ambient Monitoring

Model : EC9850

Serial Number : 02-0314

Calibration Standard equipment : Std. Gas Mixture Cylinder Number EB0140749 Expired Date 10-Mar-2024

Brand : Airgas

Components

Carbon Monoxide (CO)
Nitric Oxide (NO)
Sulfur Dioxide (SO₂)
Nitrogen (N₂)

Concentration

4498 PPM
45.69 PPM
45.54 PPM
Balance

Calibration Setting

Span Instrument Gain 25.833

Start Time 11:00

Reading (Before Adj.)			
Span Set Point	Expected Concentration (PPB)	Analyzer Response (PPB)	Error %
Zero	0	0	-
Span	400	400	0.00

Span Instrument Gain 26.634

Finish Time 11:35

Signature

Approved

บริษัท สิทธิพรแอสโซซิเอต จำกัด
SITHIPORN ASSOCIATES COMPANY LIMITED

CERTIFICATE OF ANALYSIS

Grade of Product: EPA Protocol

Part Number:	E04NI99E15A00V3	Reference Number:	160-402036564-1
Cylinder Number:	EB0140749	Cylinder Volume:	144.4 CF
Laboratory:	124 - Plumsteadville - PA	Cylinder Pressure:	2015 PSIG
PGVP Number:	A12021	Valve Outlet:	660
Gas Code:	CO,NO,NOX,SO2,BALN	Certification Date:	Mar 10, 2021

Expiration Date: Mar 10, 2024

Certification performed in accordance with "EPA Traceability Protocol for Assay and Certification of Gaseous Calibration Standards (May 2012)" document EPA 600/R-12/531, using the assay procedures listed. Analytical Methodology does not require correction for analytical interference. This cylinder has a total analytical uncertainty as stated below with a confidence level of 95%. There are no significant impurities which affect the use of this calibration mixture. All concentrations are on a mole/mole basis unless otherwise noted.

Do Not Use This Cylinder below 100 psig, i.e. 0.7 megapascals.

ANALYTICAL RESULTS					
Component	Requested Concentration	Actual Concentration	Protocol Method	Total Relative Uncertainty	Assay Dates
NOX	45.00 PPM	45.70 PPM	G1	+/- 1.1% NIST Traceable	03/03/2021, 03/10/2021
NITRIC OXIDE	45.00 PPM	45.69 PPM	G1	+/- 1.1% NIST Traceable	03/03/2021, 03/10/2021
SULFUR DIOXIDE	45.00 PPM	45.54 PPM	G1	+/- 1.1% NIST Traceable	03/03/2021, 03/10/2021
CARBON MONOXIDE	4500 PPM	4498 PPM	G1	+/- 0.6% NIST Traceable	03/04/2021
NITROGEN	Balance				

CALIBRATION STANDARDS					
Type	Lot ID	Cylinder No	Concentration	Uncertainty	Expiration Date
NTRM	200611-04	CC707968	49.82 PPM NITRIC OXIDE/NITROGEN	+/-1.0%	Feb 02, 2025
PRM	12386	D685025	9.91 PPM AIR/NITROGEN DIOXIDE	2.0%	Feb 20, 2020
GMIS	124206889	CC323707	4.028 PPM NITROGEN DIOXIDE/NITROGEN	2.1%	Aug 15, 2021
NTRM	0141709	KAL003190	49.67 PPM SULFUR DIOXIDE/NITROGEN	+/- 1.0%	Jun 20, 2022
NTRM	08012341	KAL004716	4857 PPM CARBON MONOXIDE/NITROGEN	+/- 0.6%	Jun 07, 2024

The SRM, PRM or RGM noted above is only in reference to the GMIS used in the assay and not part of the analysis.

ANALYTICAL EQUIPMENT		
Instrument/Make/Model	Analytical Principle	Last Multipoint Calibration
SIEMENS ULTRAMAT 6 N1KD579	NDIR	Feb 26, 2021
Nicolet iS50 FTIR AUP2010245 NO	FTIR	Feb 11, 2021
Nicolet iS50 FTIR AUP2010245 NO2	FTIR	Feb 22, 2021
Nicolet iS50 FTIR AUP2010245 SO2	FTIR	Feb 18, 2021

Triad Data Available Upon Request

NOTES:

Gross Weight: 28.4 Kg
Net Weight: 4.6 Kg
PO# 5221000722




Approved for Release

TEST REPORT

CUSTOMER NAME : All-Quip Co., Ltd. [บริษัท ออล คิวป์ จำกัด (สำนักงานใหญ่)]			
EQUIPMENT NAME : SO ₂ Analyzer			
MANUFACTURER : HORIBA	MODEL : APSA-370	SERIAL NO : YAW9F92K	
STANDARD GAS CONCENTRATION (PPM) : 53.29 PPM		CYLINDER NO : CC734373	
CYLINDER PRESSURE (PSI) : 1,400 PSI		CERTIFIED DATE : 12/05/2020	
CERTIFIED BY : AIRGAS		EXPIRED DATE : 12/05/2028	

TEST RESULTS

POINT NO	TEST RESULTS			
	IDEAL	ACTUAL	ERROR	%ERROR
ZERO	0.00	0.10	0.10	-
1	100.00	102.00	2.0	2.00
2	200.00	201.90	1.9	0.95
3	300.00	301.70	1.7	0.57
4	400.00	399.90	-0.1	-0.03
AVERAGE (%)				0.87

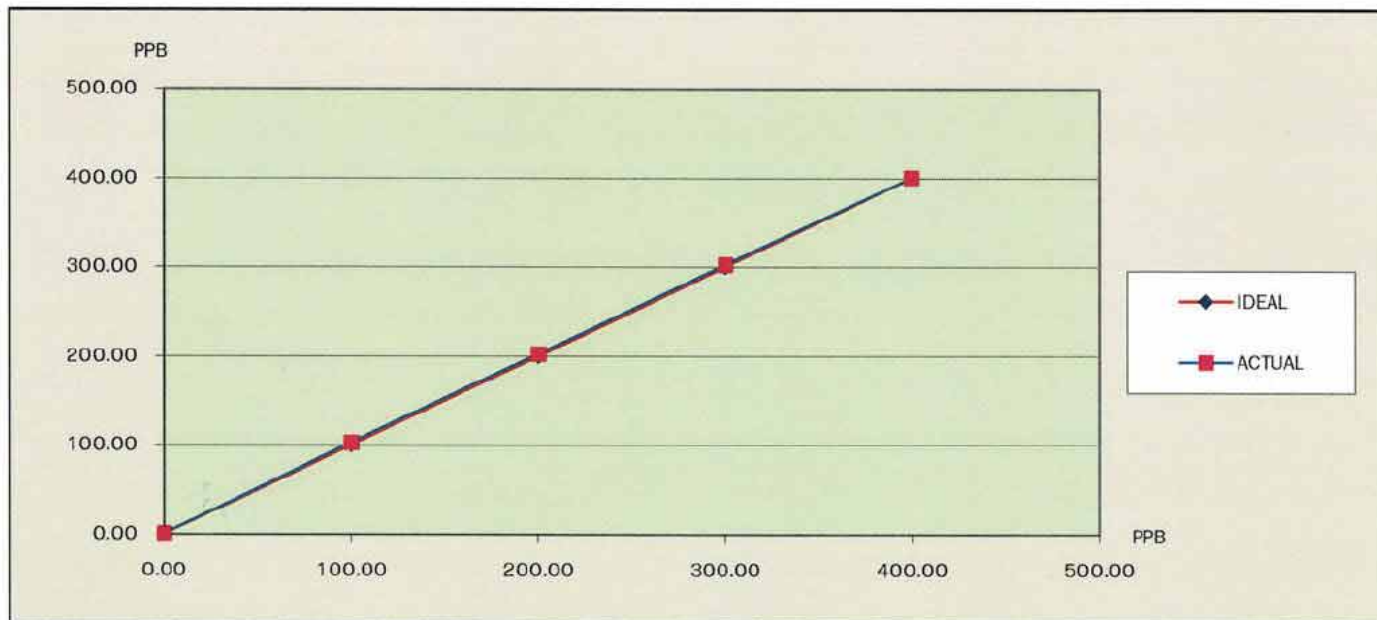

CALIBRATED BY : [REDACTED] DATE : 15/2/24

CHECKED BY : [REDACTED] DATE : 15/2/24



ต้องการข้อมูลทางด้านเทคนิคเพิ่มเติม : เจ้าหน้าที่ฝ่ายบริการหลังการขาย , โทร 02-868-0812 # 15-16 , E-Mail : Engineer@jiranatee.com

เลขที่ 63/14-15,67/35-36 ถนน ซอยเพชรเกษม 7,7/1 เพชรเกษม แขวงวัดท่าพระ เขตบางกอกใหญ่ กรุงเทพฯ 10600 โทร 02-868-0812-13 โทรสาร 02-868-1889



JIRANATEE ASSOCIATES CO.,LTD.

CHECK LIST

CUSTOMER NAME : All-Quip Co., Ltd. [บริษัท ออล ควิป จำกัด (สำนักงานใหญ่)]		
EQUIPMENT NAME : SO ₂ Analyzer		
MANUFACTURER : HORIBA	MODEL : APSA-370	SERIAL NO. : YAW9F92K

TEST VALUES				
NO.	Ambient SO ₂ Monitor	UNIT	BEFORE	AFTER
1	SIGNAL	mV (Voltage of the measured SO ₂ Value)	7.20	2.10
2	LAMP	mV (200mV to 1200 mV)	294.70	294.70
3	CELL	°C (Ambient tembient temperature +(5°C to 15°C))	35.80	35.80
4	PUMP	kPa (65 kPa or less)	41.80	41.80
5	AMBIENT	kPa	101.20	101.20
6	SAMPLE	L/min (0.6 L/min to 1.0 L/min)	-	-
7	DC 24 V	V (24 V ± 0.5 V)	23.90	23.90
8	DC 5 V	V (5 V ± 0.5 V)	5.00	5.00
9	SAMPLE SO2 Reading	PPB	1.90	0.50
10	Zero	PPB	1.90	0.10
11	Span	PPB	432.60	399.90

Remark : Reference EX-EN-019-56 , Ambient SO2 Monitor APSA-370 Operetion Manual Page #78

(Ambeint temperature = 5°C to 40°C)

อาการที่ตรวจพบ

รายละเอียดการดำเนินการ

- ทำ Calibration Zero/Span , Multipoint , เช็ค Dianostics

ผลการดำเนินการ

- เรียบร้อย เครื่องสามารถดำเนินการตรวจวัดได้ตามปกติ

CALIBRATED BY :

DATE : 15/2/24

CHECKED BY :

DATE : 15/2/24



ต้องการข้อมูลทางด้านเทคนิคเพิ่มเติม : เจ้าหน้าที่ฝ่ายบริการหลังการขาย , โทร 02-868-0812 # 15-16 , E-Mail : Engineer@jiranatee.com

เลขที่ 63/14-15 , 67/35-36 ซอยเพชรเกษม 7,7/1 ถนนเพชรเกษม แขวงวัดท่าพระ เขตบางกอกใหญ่ กรุงเทพฯ 10600 โทร : 02-868-0812-13 โทรสาร : 02-868-1889

MULTI POINT CALIBRATION REPORT

CUSTOMER NAME : บริษัท ชีวติและสิ่งแวดล้อม จำกัด

EQUIPMENT NAME : NO_x Analyzer

MANUFACTURER : Teledyne API

MODEL : 200EH

SERIAL NUMBER : 2288

STANDARD GAS CONCENTRATION (PPM) : 53.40

CYLINDER NO : CC745169

CYLINDER PRESSURE (PSIG) : 2015


CERTIFIED DATE : Mar 10, 2021

CERTIFIED BY : AIRGAS SPECIALTY GASES

EXPIRED DATE : Mar 10, 2029

CALIBRATION RESULTS

POINT NO	CALIBRATION RESULTS						
	IDEAL (PPM)	ACTUAL NO (PPM)	ERROR NO (PPM)	% ERROR NO	ACTUAL NO _x (PPM)	ERROR NO _x (PPM)	% ERROR NO _x
ZERO	0.00	0.00	0.00	-	0.00	0.00	-
1	100.00	100.30	0.30	0.30	100.30	0.30	0.30
2	200.00	203.30	3.30	1.65	203.30	3.30	1.65
3	300.00	302.00	2.00	0.67	302.00	2.00	0.67
4	400.00	399.50	-0.50	-0.13	401.50	1.50	0.38
AVERAGE (%)				0.68			0.75

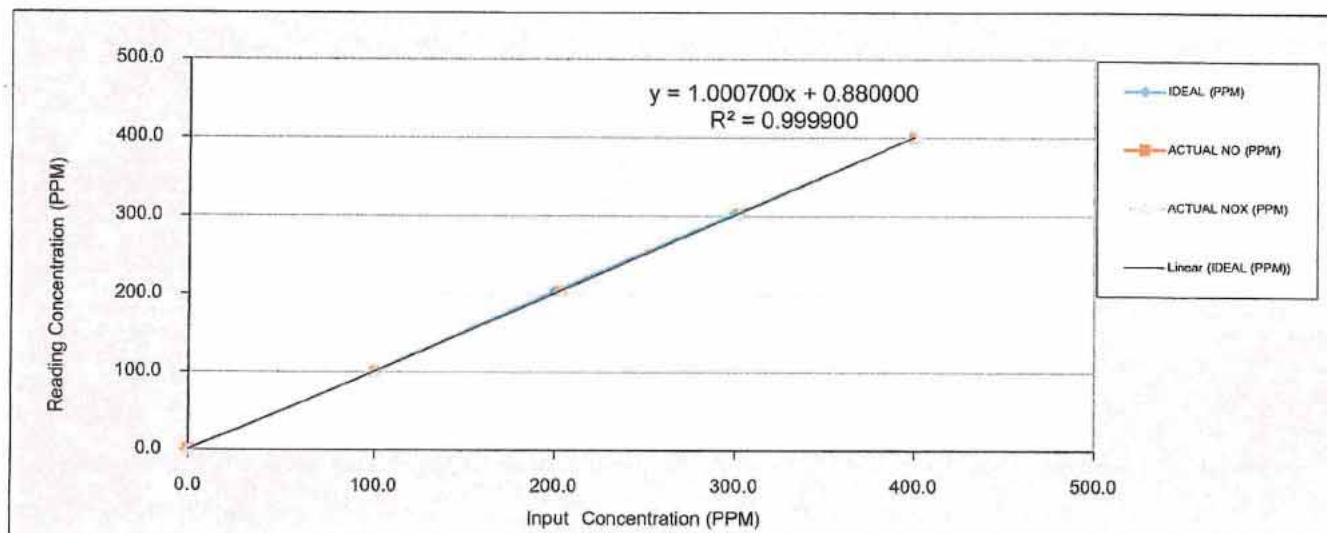

CALIBRATED BY :

DATE : 22 กุมภาพันธ์ 2567

ต้องการข้อมูลทางด้านเทคนิคเพิ่มเติม :

โทรศัพท์ : 02-515-8987

รายงานผลการซ่อมและปรับเทียบอุปกรณ์ตรวจวัดคุณภาพอากาศ

ลูกค้า / หน่วยงาน : บริษัท ซีวีดีและสิ่งแวดล้อม จำกัด

วันที่ : 22 กุมภาพันธ์ 2567

รายชื่ออุปกรณ์ / เครื่องมือ : NO_x Analyzer

บริษัทผู้ผลิต : Teledyne API

รุ่นของอุปกรณ์ / เครื่องมือ : 200E

หมายเลขอุปกรณ์ / เครื่องมือ : 2288

TEST VALUES

API MODEL 200E			BEFORE	AFTER
1	RANGE	50 - 20,000 PPM	500.0	500
2	STABILITY	≤ 1 PPM	0.4	0.1
3	SAMPLE FLOW	500 ± 10% cc/min	489	488
4	OZONE FLOW	80 ± 10% cc/min	80	80
5	PMT	mV	53.2	62
6	NORM PMT	mV	3.9	23.3
7	A ZERO	-20 To 150 mV	58	49.2
8	HPVS	400 - 900 V	762	750
9	RX CELL TEMP	50 ± 1 °C	49.9	50.0
10	BOX TEMP	AMBIENT ± 5 °C	29.3	32.4
11	PMT TEMP	7 ± 2 °C	6.9	6.9
12	MOLY TEMP	315 ± 5 °C	314	314
13	RX CELL PRESSURE	< 10 in - Hg-A	5.1	5.0
14	SAMPLE PRESSURE	25 - 35 in - Hg-A	29.6	29.5
15	NOX SLOPE	1.0 ± 0.3	1.245	1.131
16	NOX OFFSET	-50 To 150	24.2	14.2
17	NO SLOPE	1.0 ± 0.3	1.117	1.024
18	NO OFFSET	-50 To 150	1.3	1.1
19	NO SAMPLE READING	PPM	1.6	0.6
20	NO2 SAMPLE READING	PPM	7.0	6.5
21	NOX SAMPLE READING	PPM	8.6	7.1
22	OPTIC TEST	2000 ± 1000 mV	1972	1980
23	ELECTRICAL TEST	2000 ± 1000 mV	2153	2150
24	VOLTAGE TEST	+5 V +12 V +15 V -15 V	5.21 / 12.23 / 15.69 / -15.14	5.21 / 12.17 / 15.99 / -15.11
25	ZERO GAS NO / NOx	0.00 / 0.00 PPM	0.1 / -5.2	0.0 / 0.0
26	SPAN GAS NO / NOx	400.00 / 400.00 PPM	418 / 430	399.5 / 401.5

หมายเหตุ

- ทำการเปลี่ยน OZONE GENERATOR นำเอาของเครื่อง Nox Sn.2287 มาใส่แทน เนื่องจากตัวเก่าของเครื่องใช้งานไม่ได้
- Calibrate Multi-point


ลงนามเจ้าหน้าที่ (Signature)

Test Report Calibration

Ecotech EC9841 Nitrogen Oxides Analyzer

Issued By	Sithiporn Associates Company Limited	Calibration Date	22-Jan-2024
Owner Name	Life & Environment Co.,Ltd.	Product Brand	Ecotech
Certificate Number	34303	Type Systematic	Analyzer Ambient Monitoring

Model : EC9841

Serial Number : 02-0409

Calibration Standard equipment : Std. Gas Mixture Cylinder Number EB0140749 Expired Date 10-Mar-2024

Brand : Airgas

Components

Carbon Monoxide (CO)

Nitric Oxide (NO)

Sulfur Dioxide (SO₂)Nitrogen (N₂)

Concentration

4498 PPM

45.69 PPM

45.54 PPM

Balance

Calibration Setting

Span Instrument Gain 13.546

Start Time 11:00

Reading (After Adj.)			
Span Set Point	Expected Concentration (PPB)	Analyzer Response (PPB)	Error %
Zero NO	0	0	-
Zero NO _x	0	1	-
Span NO	400	399	-0.25
Span NO _x	400	400	0.00

Span Instrument Gain 10.764

Finish Time 11:35

Signature

Approved

บริษัท สิทธิพรแอสโซซิเอต จำกัด

SITHIPORN ASSOCIATES COMPANY LIMITED

CERTIFICATE OF ANALYSIS

Grade of Product: EPA Protocol

Part Number:	E04NI99E15A00V3	Reference Number:	160-402036564-1
Cylinder Number:	EB0140749	Cylinder Volume:	144.4 CF
Laboratory:	124 - Plumsteadville - PA	Cylinder Pressure:	2015 PSIG
PGVP Number:	A12021	Valve Outlet:	660
Gas Code:	CO,NO,NOX,SO2,BALN	Certification Date:	Mar 10, 2021

Expiration Date: Mar 10, 2024

Certification performed in accordance with "EPA Traceability Protocol for Assay and Certification of Gaseous Calibration Standards (May 2012)" document EPA 600/R-12/531, using the assay procedures listed. Analytical Methodology does not require correction for analytical interference. This cylinder has a total analytical uncertainty as stated below with a confidence level of 95%. There are no significant impurities which affect the use of this calibration mixture. All concentrations are on a mole/mole basis unless otherwise noted.

Do Not Use This Cylinder below 100 psig, i.e. 0.7 megapascals.

ANALYTICAL RESULTS					
Component	Requested Concentration	Actual Concentration	Protocol Method	Total Relative Uncertainty	Assay Dates
NOX	45.00 PPM	45.70 PPM	G1	+/- 1.1% NIST Traceable	03/03/2021, 03/10/2021
NITRIC OXIDE	45.00 PPM	45.69 PPM	G1	+/- 1.1% NIST Traceable	03/03/2021, 03/10/2021
SULFUR DIOXIDE	45.00 PPM	45.54 PPM	G1	+/- 1.1% NIST Traceable	03/03/2021, 03/10/2021
CARBON MONOXIDE	4500 PPM	4498 PPM	G1	+/- 0.6% NIST Traceable	03/04/2021
NITROGEN	Balance				

CALIBRATION STANDARDS					
Type	Lot ID	Cylinder No	Concentration	Uncertainty	Expiration Date
NTRM	200611-04	CC707968	49.82 PPM NITRIC OXIDE/NITROGEN	+/-1.0%	Feb 02, 2025
PRM	12386	D685025	9.91 PPM AIR/NITROGEN DIOXIDE	2.0%	Feb 20, 2020
GMIS	124206889	CC323707	4.028 PPM NITROGEN DIOXIDE/NITROGEN	2.1%	Aug 15, 2021
NTRM	0141709	KAL003190	49.67 PPM SULFUR DIOXIDE/NITROGEN	+/- 1.0%	Jun 20, 2022
NTRM	08012341	KAL004716	4857 PPM CARBON MONOXIDE/NITROGEN	+/- 0.6%	Jun 07, 2024

The SRM, PRM or RGM noted above is only in reference to the GMIS used in the assay and not part of the analysis.

ANALYTICAL EQUIPMENT		
Instrument/Make/Model	Analytical Principle	Last Multipoint Calibration
SIEMENS ULTRAMAT 6 N1KD579	NDIR	Feb 26, 2021
Nicolet iS50 FTIR AUP2010245 NO	FTIR	Feb 11, 2021
Nicolet iS50 FTIR AUP2010245 NO2	FTIR	Feb 22, 2021
Nicolet iS50 FTIR AUP2010245 SO2	FTIR	Feb 18, 2021

Triad Data Available Upon Request

NOTES:

Gross Weight: 28.4 Kg
Net Weight: 4.6 Kg
PO# 5221000722



[Redacted Signature]

Approved for Release




TEST REPORT

CUSTOMER NAME	: All-Quip Co., Ltd. [บริษัท ออล ควิป จำกัด (สำนักงานใหญ่)]						
EQUIPMENT NAME	: NO _x Analyzer						
MANUFACTURER	: HORIBA	MODEL :	APNA-370	SERIAL NO	: J0V032W3		
STANDARD GAS CONCENTRATION (PPM)	: 53.15 PPM			CYLINDER NO	: CC734373		
CYLINDER PRESSURE (PSI)	: 1,400 PSI			CERTIFIED DATE	: 12/05/2020		
CERTIFIED BY	: AIRGAS			EXPIRED DATE	: 12/05/2028		


TEST RESULTS

POINT NO	TEST RESULTS						
	IDEAL	ACTUAL NO	ERROR NO	%ERROR NO	ACTUAL NO _x	ERROR NO _x	%ERROR NO _x
ZERO	0.00	0.40	0.40	-	0.00	0.00	-
1	100.00	101.00	1.00	1.00	100.30	0.30	0.30
2	200.00	200.80	0.80	0.40	200.50	0.50	0.25
3	300.00	301.40	1.40	0.47	300.20	0.20	0.07
4	400.00	399.60	-0.40	-0.10	399.70	-0.30	-0.08
AVERAGE (%)				0.44			0.14

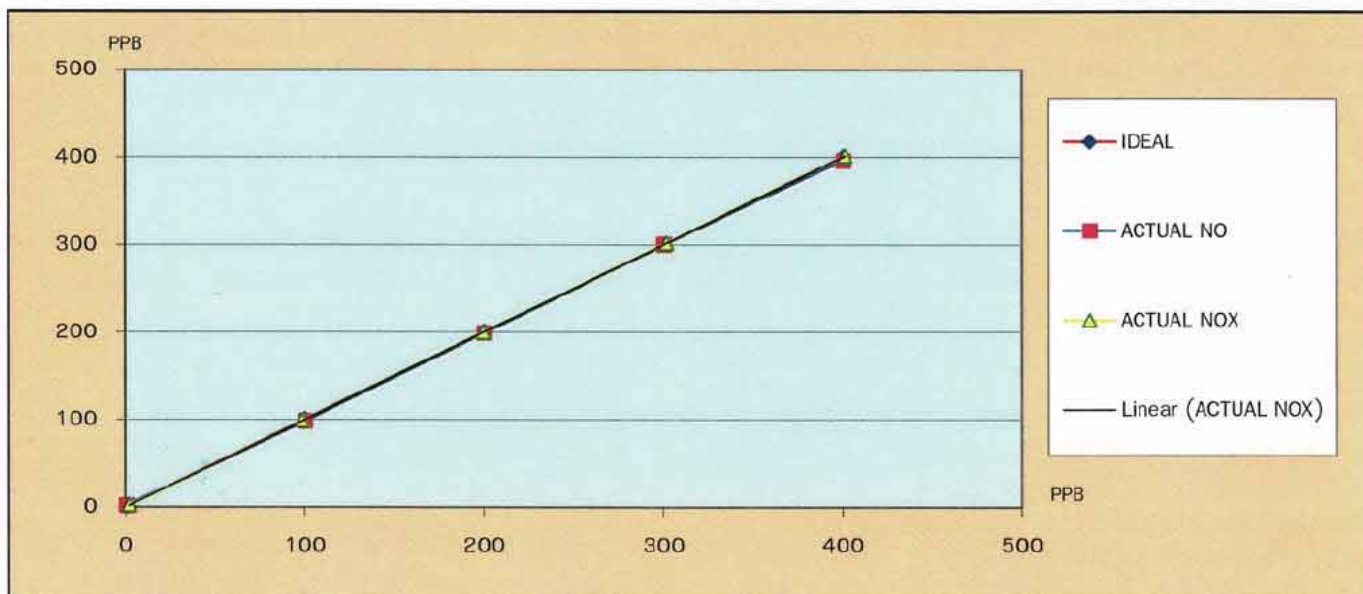

CALIBRATED BY : [REDACTED] DATE : 16/2/24

CHECKED BY : [REDACTED] DATE : 16/2/24

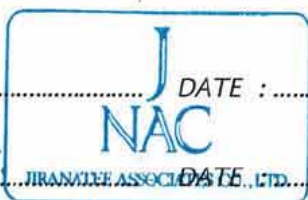

ต้องการข้อมูลทางด้านเทคนิคเพิ่มเติม : เจ้าหน้าที่ฝ่ายบริการหลังการขาย โทร 02-868-0812 # 15,16 , E-Mail : Engineer@jiranatee.com

เลขที่ 63/14-15,67/35-36 ซอยนพพรเกษม 7,7/1 ถนนเพชรเกษม แขวงวัดท่าพระ เขตบางกอกใหญ่ กรุงเทพฯ 10600 โทร 02-868-0812-13 โทรสาร 02-868-1889

CHECK LIST

CUSTOMER NAME : All-Quip Co., Ltd. [บริษัท ออล คิวิป จำกัด (สำนักงานใหญ่)]		
EQUIPMENT NAME : NO _x Analyzer		
MANUFACTURER : HORIBA	MODEL : APNA-370	SERIAL NO. : J0V032W3

TEST VALUES

NO.	NO _x Analyzer (APNA-370)	UNIT	BEFORE	AFTER
1	Signal (NO)	mV	1.60	1.30
2	Signal (NO _x)	mV	6.00	12.60
3	Detector	Temp °C , Standard Value : Ambient temp+(5°Cto15°C)	42.10	40.10
		Pressure kPa , Standard Value : (Ambient/1013x100-20)±4kPa	75.80	77.90
4	AMBIENT	kPa	101.60	101.70
5	SAMPLE	L/min (1.1 L/min ± 0.3 L/min)	-	-
6	DC 24 V	V (24 V ± 0.5 V)	23.60	23.60
7	DC 5 V	V (5 V ± 0.5 V)	5.00	5.00
8	Sampling NO Reading	PPB	1.40	2.20
9	Sampling NO ₂ Reading	PPB	5.20	19.40
10	Sampling NO _x Reading	PPB	6.70	21.80
11	Zero (NO)	PPB	1.40	0.40
12	Span(NO)	PPB	389.00	399.60
13	Zero (NO _x)	PPB	1.40	0.00
14	Span (NO _x)	PPB	390.10	399.70

Remark : Reference EX-EN-022-56 , "Ambient NO_x Monitor APNA-370 Operation Manual " Page #48

(Ambient temperature = 5°C to 40°C)

อาการที่ตรวจพบ

- Touch Screen ไม่ได้

รายละเอียดการดำเนินการ

- เปลี่ยน Touch Screen ทำ Calibration Zero/Span , Multipoint , เช็ค Diagnostics

ผลการดำเนินการ

- เรียบร้อย เครื่องสามารถดำเนินการตรวจวัดได้ตามปกติ

CALIBRATED BY :

DATE : 16/2/24

CHECKED BY :

DATE : 16/2/24

ต้องการข้อมูลทางด้านเทคนิคเพิ่มเติม : เจ้าหน้าที่ฝ่ายบริการหลังการขาย , โทร 02-868-0812 # 15-16 , E-Mail : Engineer@jiranatee.com

เลขที่ 63/14-15,67/35-36 ซอยเพชรเกษม 7,7/1 ถนนเพชรเกษม แขวงวัดท่าพระ เขตบางกอกใหญ่ กรุงเทพฯ 10600 โทร 02-868-0812-13 โทรสาร 02-868-1889

Maintenance and Calibration Report

Wind Speed Sensor

Met One Instrument	Model: 034B	S/N. : Y1846
Date 7 February 2024		Start Time 13:30
Calibrator : Metone	Model: 053-220	S/N.: W15225
Data Logger : Metone	Model: 466A	S/N.: Y1191

Customer : Life & Environment Co.,Ltd.

Maintenance

Replace Front Bearing	<input type="checkbox"/> Yes	<input checked="" type="checkbox"/> No
Replace Back Bearing	<input type="checkbox"/> Yes	<input checked="" type="checkbox"/> No
Replace Shaft Coupler	<input type="checkbox"/> Yes	<input checked="" type="checkbox"/> No
Replace Hub	<input type="checkbox"/> Yes	<input checked="" type="checkbox"/> No

Testing Result

Generate Speed	Reading		% Error
RPM	Expect (MPS)	Logger	
0	0.30	0.30	0.0
100	2.94	3.10	-5.4
200	5.61	5.50	2.0
300	8.27	8.30	-0.4
400	10.93	11.10	-1.6
500	13.60	13.50	0.7

Comment : Set the offset of WS is 0.3 m/s.

Test by force to rotate the WS sensor from 0 - 500 round per second.

Data Logger Metone Model 466A, S/N. Y1191

Engineer Name :

Maintenance and Calibration Report

Wind Direction Sensor

Met One Instrument

Model: 034B

S/N. : Y1846

Date 7 February 2024

Start Time 13:30

Data Logger : Metone

Model: 466A

S/N.: Y1191

Customer : Life & Environment Co.,Ltd.

Maintenance

Replace Front Bearing

☐ Yes ☒ No

Replace Back Bearing

☐ Yes ☒ No

Replace Potentiometer

☐ Yes ☒ No

Calibration Result

Reading			Analog Output (Volt)	
Expected	Logger	% Error	Expected	Measured
360,0	0.1	0.1	2.500	2.499
90	90.1	0.1	0.625	0.625
180	180.0	0.0	1.250	1.249
270	270.0	0.0	1.875	1.874

Comment : Check the rotation of WD (potentiometer) is change as characteristic.

Performed rotate the WD increase 90 degree per 1 step from 0,360 , 90, 180 and 270 degree.

Data Logger Metone Model 466A, S/N. Y1191

Engineer Name : 



Certificate of Calibration

Page : 1 of 3

90, 92, 94 Soi On-Nuch 64, Srinakarin Rd., On-Nuch, Suanluang,
Bangkok 10250

ID. Number : N/A

Date of Issue : 02 Mar 2024

The calibration certificate shall not be reproduced except in full, without written approval of SP Metrology System (Thailand).

Approved by : [REDACTED]

(Mr.

Authorized Signatory



ID LINE : IEC17025



Calibration Report

Certificate Number : SPR24020474-8

Page : 2 of 3


Reference Standards

Equipment Name	Model	Serial No.	Certificate No.	Due. Date
Sound Level Calibrator	ST-120	211203773	EEL.BP. 140/0167	26 Jan 2025

Traceability

This certification is traceable to the International System of Unit maintained at :

TISTR - Thailand Institute of Scientific and Technological Research



Certificate No. : SPR24020474-8

Range : 94 to 114 dB

Function : @1kHz

Unit : dB

Select	C	Unit : dB			
Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	93.7	93.7	-0.3	-0.3	0.15
114	113.7	113.7	-0.3	-0.3	0.15

Unit : dB

Note:

The result of calibration was found accurate as show on date and place of calibration only.
This Certificate is not certified for any commercial transaction.

Measurement Uncertainty

The reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor $k = 2.00$, providing a level of confidence approximately 95%.

- End of Certificate -



ID LINE : IEC17025



Certificate of Calibration

Certificate Number : SPR24020474-9

Page : 1 of 3

Customer : Life and Environment Co., Ltd.

90, 92, 94 Soi On-Nuch 64, Srinakarin Rd., On-Nuch, Suanluang,
Bangkok 10250

Equipment Name : Sound Level Meter

Manufacturer : Pulsar

Model : 45

Serial Number : PN2450

ID. Number : N/A

Environmental Conditions

Ambient Temperature : $23^{\circ}\text{C} \pm 3^{\circ}\text{C}$ Received Date : 29 Feb 2024

Relative Humidity : $50\% \pm 15\%$ Calibration Date : 01 Mar 2024

Location of Calibration : In-Lab Recommend Due Date : 01 Mar 2025

Calibration Procedure : SP-CPE-04-01 Date of Issue : 02 Mar 2024

Method of Calibration

This certifies that the above instrument was calibrated in compliance with the calibration system requirement of ISO/IEC 17025:2017 in accordance with reference procedure. Standards used to perform this calibration are certified by to NIST or equivalent, National metrology institute, Natural physical constants, consensus standards. The result reported herein apply only to the calibration of the item described above as received. Our decision rule is to contact the customer if the item pass and fail calibration when the results include the uncertainties and the customer must determine if the results meets their needs.

The calibration certificate shall not be reproduced except in full, without written approval of SP Metrology System (Thailand).

Calibrated by :



Calibration Officer

Approved by :



Authorized Signatory



ID LINE : IEC17025



Calibration Report

Certificate Number : SPR24020474-9

Page : 2 of 3

Reference Standards

Equipment Name	Model	Serial No.	Certificate No.	Due. Date
Sound Level Calibrator	ST-120	211203773	EEL.BP. 140/0167	26 Jan 2025

Traceability

This certification is traceable to the International System of Unit maintained at :

TISTR - Thailand Institute of Scientific and Technological Research



ID LINE : IEC17025



Result of Calibration

Certificate No. : SPR24020474-9

Page : 3 of 3

Range : 94 to 114 dB

Function : @1kHz

Select A

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	93.7	93.7	-0.3	-0.3	0.15
114	113.6	113.6	-0.4	-0.4	0.15

Select C

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	93.7	93.7	-0.3	-0.3	0.15
114	113.6	113.6	-0.4	-0.4	0.15

Select Z

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	93.7	93.7	-0.3	-0.3	0.15
114	113.6	113.6	-0.4	-0.4	0.15

Note:

The result of calibration was found accurate as show on date and place of calibration only.
This Certificate is not certified for any commercial transaction.

Measurement Uncertainty

The reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor $k = 2.00$, providing a level of confidence approximately 95%.

- End of Certificate -



ID LINE : IEC17025



Certificate of Calibration

Certificate Number : SPR24020474-10

Page : 1 of 3

Customer : Life and Environment Co., Ltd.

90, 92, 94 Soi On-Nuch 64, Srinakarin Rd., On-Nuch, Suanluang,
Bangkok 10250

Equipment Name : Sound Level Meter

Manufacturer : Pulsar

Model : 45

Serial Number : PN2451

ID. Number : N/A

Environmental Conditions

Ambient Temperature : $23^{\circ}\text{C} \pm 3^{\circ}\text{C}$

Received Date : 29 Feb 2024

Relative Humidity : $50\% \pm 15\%$

Calibration Date : 01 Mar 2024

Location of Calibration : In-Lab

Recommend Due Date : 01 Mar 2025


Calibration Procedure : SP-CPE-04-01

Date of Issue : 02 Mar 2024


Method of Calibration

This certifies that the above instrument was calibrated in compliance with the calibration system requirement of ISO/IEC 17025:2017 in accordance with reference procedure. Standards used to perform this calibration are certified by to NIST or equivalent, National metrology institute, Natural physical constants, consensus standards. The result reported herein apply only to the calibration of the item described above as received. Our decision rule is to contact the customer if the item pass and fail calibration when the results include the uncertainties and the customer must determine if the results meets their needs.

The calibration certificate shall not be reproduced except in full, without written approval of SP Metrology System (Thailand).

Calibrated by : 
Calibration Officer

Approved by :


Authorized Signatory



ID LINE : IEC17025



Calibration Report

Certificate Number : SPR24020474-10

Page : 2 of 3

Reference Standards

Equipment Name	Model	Serial No.	Certificate No.	Due. Date
Sound Level Calibrator	ST-120	211203773	EEL.BP. 140/0167	26 Jan 2025

Traceability

This certification is traceable to the International System of Unit maintained at :

TISTR - Thailand Institute of Scientific and Technological Research



ID LINE : IEC17025



Result of Calibration

Certificate No. : SPR24020474-10

Page : 3 of 3

Range : 94 to 114 dB

Function : @1kHz

Select A

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	93.7	93.7	-0.3	-0.3	0.15
114	113.6	113.6	-0.4	-0.4	0.15

Select C

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	93.7	93.7	-0.3	-0.3	0.15
114	113.6	113.6	-0.4	-0.4	0.15

Select Z

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	93.7	93.7	-0.3	-0.3	0.15
114	113.6	113.6	-0.4	-0.4	0.15

Note:

The result of calibration was found accurate as show on date and place of calibration only.
This Certificate is not certified for any commercial transaction.

Measurement Uncertainty

The reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor $k = 2.00$, providing a level of confidence approximately 95%.

- End of Certificate -



ID LINE : IEC17025



Certificate of Calibration

Certificate Number : SPR24050563-1

Page : 1 of 3

Customer : Life and Environment Co., Ltd.

90, 92, 94 Soi On-Nuch 64, Srinakarin Rd., On-Nuch, Suanluang,
Bangkok 10250

Equipment Name : Sound Level Meter

Manufacturer : ACO

Model : 6236

Serial Number : 222219

ID. Number : SLM-NO.8

Environmental Conditions

Ambient Temperature : $23^{\circ}\text{C} \pm 3^{\circ}\text{C}$

Received Date : 31 May 2024

Relative Humidity : $50\% \pm 15\%$

Calibration Date : 05 Jun 2024

Location of Calibration : In-Lab

Recommend Due Date : 05 Jun 2025

Calibration Procedure : SP-CPE-04-01

Date of Issue : 06 Jun 2024

Method of Calibration

This certifies that the above instrument was calibrated in compliance with the calibration system requirement of ISO/IEC 17025:2017 in accordance with reference procedure. Standards used to perform this calibration are certified by to NIST or equivalent, National metrology institute, Natural physical constants, consensus standards. The result reported herein apply only to the calibration of the item described above as received. Our decision rule is to contact the customer if the item pass and fail calibration when the results include the uncertainties and the customer must determine if the results meets their needs.

The calibration certificate shall not be reproduced except in full, without written approval of SP Metrology System (Thailand).

Calibrated by :



Calibration Officer

Approved by :



Authorized Signatory



ID LINE : IEC17025



Calibration Report

Certificate Number : SPR24050563-1

Page : 2 of 3

Reference Standards

Equipment Name	Model	Serial No.	Certificate No.	Due. Date
Sound Level Calibrator	ST-120	211203773	EEL.BP. 140/0167	26 Jan 2025

Traceability

This certification is traceable to the International System of Unit maintained at :
TISTR - Thailand Institute of Scientific and Technological Research



Result of Calibration

Page : 3 of 3

Function : @1kHz

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.0	93.9	0.0	-0.1	0.15
114	113.9	113.9	-0.1	-0.1	0.15

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.0	94.0	0.0	0.0	0.15
114	113.9	113.9	-0.1	-0.1	0.15

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.0	94.0	0.0	0.0	0.15
114	113.8	113.8	-0.2	-0.2	0.15


Note:

The result of calibration was found accurate as show on date and place of calibration only.
This Certificate is not certified for any commercial transaction.

Measurement Uncertainty

The reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor $k = 2.00$, providing a level of confidence approximately 95%.

- End of Certificate -



Certificate of Calibration

Page : 1 of 3

90, 92, 94 Soi On-Nuch 64, Srinakarin Rd., On-Nuch, Suanluang,
Bangkok 10250

ID. Number : SLM-NO.9

Date of Issue : 06 Jun 2024

The calibration certificate shall not be reproduced except in full, without written approval of SP Metrology System (Thailand).

Calibration Officer



Authorized Signatory



ID LINE : IEC17025



Calibration Report

Certificate Number : SPR24050563-2

Page : 2 of 3

Reference Standards

Equipment Name	Model	Serial No.	Certificate No.	Due. Date
Sound Level Calibrator	ST-120	211203773	EEL.BP. 140/0167	26 Jan 2025

Traceability

This certification is traceable to the International System of Unit maintained at :

TISTR - Thailand Institute of Scientific and Technological Research



ID LINE : IEC17025



Result of Calibration

Certificate No. : SPR24050563-2

Page : 3 of 3

Range : 94 to 114 dB

Function : @1kHz

Select A

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.0	93.9	0.0	-0.1	0.15
114	113.9	113.9	-0.1	-0.1	0.15

Select C

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.0	94.0	0.0	0.0	0.15
114	113.8	113.8	-0.2	-0.2	0.15

Select Z

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.0	94.0	0.0	0.0	0.15
114	113.8	113.8	-0.2	-0.2	0.15

Note:

The result of calibration was found accurate as show on date and place of calibration only.
This Certificate is not certified for any commercial transaction.

Measurement Uncertainty

The reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor $k = 2.00$, providing a level of confidence approximately 95%.

- End of Certificate -



ID LINE : IEC17025



Certificate of Calibration

Certificate Number : SPR24050563-3

Page : 1 of 3

Customer : Life and Environment Co., Ltd.

90, 92, 94 Soi On-Nuch 64, Srinakarin Rd., On-Nuch, Suanluang,
Bangkok 10250

Equipment Name : Sound Level Meter

Manufacturer : ACO

Model : 6236

Serial Number : 222222

ID. Number : SLM-NO.11

Environmental Conditions

Ambient Temperature : $23^{\circ}\text{C} \pm 3^{\circ}\text{C}$

Received Date : 31 May 2024

Relative Humidity : $50\% \pm 15\%$

Calibration Date : 05 Jun 2024

Location of Calibration : In-Lab

Recommend Due Date : 05 Jun 2025

Calibration Procedure : SP-CPE-04-01

Date of Issue : 06 Jun 2024

Method of Calibration

This certifies that the above instrument was calibrated in compliance with the calibration system requirement of ISO/IEC 17025:2017 in accordance with reference procedure. Standards used to perform this calibration are certified by to NIST or equivalent, National metrology institute, Natural physical constants, consensus standards. The result reported herein apply only to the calibration of the item described above as received. Our decision rule is to contact the customer if the item pass and fail calibration when the results include the uncertainties and the customer must determine if the results meets their needs.

The calibration certificate shall not be reproduced except in full, without written approval of SP Metrology System (Thailand).

Calibrated by :



Calibration Officer

Approved by :



Authorized Signatory



ID LINE : IEC17025



Calibration Report

Certificate Number : SPR24050563-3

Page : 2 of 3

Reference Standards

Equipment Name	Model	Serial No.	Certificate No.	Due. Date
Sound Level Calibrator	ST-120	211203773	EEL.BP. 140/0167	26 Jan 2025

Traceability

This certification is traceable to the International System of Unit maintained at :

TISTR - Thailand Institute of Scientific and Technological Research



ID LINE : IEC17025



Result of Calibration

Certificate No. : SPR24050563-3

Page : 3 of 3

Range : 94 to 114 dB

Function : @1kHz

Select A

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.0	94.0	0.0	0.0	0.15
114	113.8	113.8	-0.2	-0.2	0.15

Select C

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.0	94.0	0.0	0.0	0.15
114	113.8	113.8	-0.2	-0.2	0.15

Select Z

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.0	94.0	0.0	0.0	0.15
114	113.8	113.8	-0.2	-0.2	0.15

Note:

The result of calibration was found accurate as show on date and place of calibration only.
This Certificate is not certified for any commercial transaction.

Measurement Uncertainty

The reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor $k = 2.00$, providing a level of confidence approximately 95%.

- End of Certificate -



ID LINE : IEC17025



Certificate of Calibration

Certificate Number : SPR24090384-1

Page : 1 of 3

Customer : Life and Environment Co., Ltd.

90, 92, 94 Soi On-Nuch 64, Srinakarin Rd., On-Nuch, Suanluang,
Bangkok 10250

Equipment Name : Sound Level Meter

Manufacturer : ACO

Model : 6236

Serial Number : 222241

ID. Number : SLM-NO.12

Environmental Conditions

Ambient Temperature : $23^{\circ}\text{C} \pm 3^{\circ}\text{C}$

Relative Humidity : $50\% \pm 15\%$

Location of Calibration : In-Lab

Calibration Procedure : SP-CPE-04-01

Received Date : 20 Sep 2024

Calibration Date : 20 Sep 2024

Recommend Due Date : N/A

Date of Issue : 21 Sep 2024

Method of Calibration

This certifies that the above instrument was calibrated in compliance with the calibration system requirement of ISO/IEC 17025:2017 in accordance with reference procedure. Standards used to perform this calibration are certified by to NIST or equivalent, National metrology institute, Natural physical constants, consensus standards. The result reported herein apply only to the calibration of the item described above as received. Our decision rule is to contact the customer if the item pass and fail calibration when the results include the uncertainties and the customer must determine if the results meets their needs.


The calibration certificate shall not be reproduced except in full, without written approval of SP Metrology System (Thailand).

Calibrated by :



Calibration Officer

Approved by

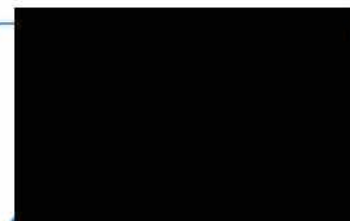

Authorized Signatory



ID LINE : IEC17025



Calibration Report

Certificate Number : SPR24090384-1

Page : 2 of 3

Reference Standards

Equipment Name	Model	Serial No.	Certificate No.	Due. Date
Sound Level Calibrator	ST-120	211203773	EEL.BP. 140/0167	26 Jan 2025

Traceability

This certification is traceable to the International System of Unit maintained at :

TISTR - Thailand Institute of Scientific and Technological Research



ID LINE : IEC17025



Result of Calibration

Certificate Number : SPR24090384-1

Page : 3 of 3

Range : 94 to 114 dB

Function : @1kHz

Select A

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.0	94.0	0.0	0.0	0.15
114	113.8	113.8	-0.2	-0.2	0.15

Select C

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.0	94.0	0.0	0.0	0.15
114	113.7	113.7	-0.3	-0.3	0.15

Note :

The result of calibration was found accurate as show on date and place of calibration only.
This Certificate is not certified for any commercial transaction.

Measurement Uncertainty

The reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor $k = 2.00$, providing a level of confidence approximately 95%.

- End of Certificate -



ID LINE : IEC17025



Certificate of Calibration

Certificate Number : SPR24090384-2

Page : 1 of 3

Customer : Life and Environment Co., Ltd.

90, 92, 94 Soi On-Nuch 64, Srinakarin Rd., On-Nuch, Suanluang,
Bangkok 10250

Equipment Name : Sound Level Meter

Manufacturer : ACO

Model : 6236

Serial Number : 222242

ID. Number : SLM-NO.13

Environmental Conditions

Ambient Temperature : $23\text{ }^{\circ}\text{C} \pm 3\text{ }^{\circ}\text{C}$

Relative Humidity : $50\% \pm 15\%$

Location of Calibration : In-Lab

Calibration Procedure : SP-CPE-04-01

Received Date : 20 Sep 2024

Calibration Date : 20 Sep 2024

Recommend Due Date : N/A

Date of Issue : 21 Sep 2024

Method of Calibration

This certifies that the above instrument was calibrated in compliance with the calibration system requirement of ISO/IEC 17025:2017 in accordance with reference procedure. Standards used to perform this calibration are certified by to NIST or equivalent, National metrology institute, Natural physical constants, consensus standards. The result reported herein apply only to the calibration of the item described above as received. Our decision rule is to contact the customer if the item pass and fail calibration when the results include the uncertainties and the customer must determine if the results meets their needs.

The calibration certificate shall not be reproduced except in full, without written approval of SP Metrology System (Thailand).

Calibrated by :



Calibration Officer

Approved by :



Authorized Signatory



ID LINE : IEC17025



Calibration Report

Certificate Number : SPR24090384-2

Page : 2 of 3

Reference Standards

Equipment Name	Model	Serial No.	Certificate No.	Due. Date
Sound Level Calibrator	ST-120	211203773	EEL.BP. 140/0167	26 Jan 2025

Traceability

This certification is traceable to the International System of Unit maintained at :

TISTR - Thailand Institute of Scientific and Technological Research



ID LINE : IEC17025



Result of Calibration

Certificate Number : SPR24090384-2

Page : 3 of 3

Range : 94 to 114 dB

Function : @1kHz

Select A

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.0	94.0	0.0	0.0	0.15
114	114.1	114.1	0.1	0.1	0.15

Select C

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.0	94.0	0.0	0.0	0.15
114	114.0	114.0	0.0	0.0	0.15

Note :

The result of calibration was found accurate as show on date and place of calibration only.
This Certificate is not certified for any commercial transaction.

Measurement Uncertainty

The reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor $k = 2.00$, providing a level of confidence approximately 95%.

- End of Certificate -



ID LINE: IEC17025



Certificate of Calibration

Certificate Number : SPR24040397-1

Page : 1 of 3

Customer : Life and Environment Co., Ltd.

90, 92, 94 Soi On-Nuch 64, Srinakarin Rd., On-Nuch, Suanluang,
Bangkok 10250

Equipment Name : Sound Level Meter

Manufacturer : Quest Technologies

Model : 1900

Serial Number : CC5020002

ID. Number : SLM-NO.1

Environmental Conditions

Ambient Temperature : $23^{\circ}\text{C} \pm 3^{\circ}\text{C}$

Received Date : 30 Apr 2024

Relative Humidity : $50\% \pm 15\%$

Calibration Date : 04 May 2024

Location of Calibration : In-Lab

Recommend Due Date : 04 May 2025

Calibration Procedure : SP-CPE-04-01

Date of Issue : 05 May 2024

Method of Calibration

This certifies that the above instrument was calibrated in compliance with the calibration system requirement of ISO/IEC 17025:2017 in accordance with reference procedure. Standards used to perform this calibration are certified by to NIST or equivalent, National metrology institute, Natural physical constants, consensus standards. The result reported herein apply only to the calibration of the item described above as received. Our decision rule is to contact the customer if the item pass and fail calibration when the results include the uncertainties and the customer must determine if the results meets their needs.


The calibration certificate shall not be reproduced except in full, without written approval of SP Metrology System (Thailand).

Calibrated by :



Calibration Officer

Approved by :

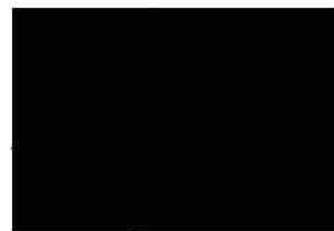

Authorized Signatory



ID LINE : IEC17025



Calibration Report

Certificate Number : SPR24040397-1

Page : 2 of 3

Reference Standards

Equipment Name	Model	Serial No.	Certificate No.	Due. Date
Sound Level Calibrator	ST-120	211203773	EEL.BP. 140/0167	26 Jan 2025

Traceability

This certification is traceable to the International System of Unit maintained at :

TISTR - Thailand Institute of Scientific and Technological Research



ID LINE : IEC17025



Result of Calibration

Certificate No. : SPR24040397-1

Page : 3 of 3

Range : 94 to 114 dB

Function : @1kHz

Select A

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.0	94.0	0.0	0.0	0.15
114	114.1	114.1	0.1	0.1	0.15

Select C

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.0	94.0	0.0	0.0	0.15
114	114.0	114.0	0.0	0.0	0.15

Note:

The result of calibration was found accurate as show on date and place of calibration only.
This Certificate is not certified for any commercial transaction.

Measurement Uncertainty

The reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor $k = 2.00$, providing a level of confidence approximately 95%.

- End of Certificate -



ID LINE : IEC17025



Certificate of Calibration

Certificate Number : SPR24060488-15

Page : 1 of 3

Customer : Life and Environment Co., Ltd.

90, 92, 94 Soi On-Nuch 64, Srinakarin Rd., On-Nuch, Suanluang,
Bangkok 10250

Equipment Name : Noise Dose Meter

Manufacturer : SOUNDTEK

Model : ST-130

Serial Number : 220100105

ID. Number : NT-07

Environmental Conditions

Ambient Temperature : $23^{\circ}\text{C} \pm 3^{\circ}\text{C}$

Received Date : 28 Jun 2024

Relative Humidity : $50\% \pm 15\%$

Calibration Date : 28 Jun 2024

Location of Calibration : In-Lab

Recommend Due Date : 28 Jun 2025

Calibration Procedure : SP-CPE-04-01

Date of Issue : 29 Jun 2024

Method of Calibration

This certifies that the above instrument was calibrated in compliance with the calibration system requirement of ISO/IEC 17025:2017 in accordance with reference procedure. Standards used to perform this calibration are certified by to NIST or equivalent, National metrology institute, Natural physical constants, consensus standards. The result reported herein apply only to the calibration of the item described above as received. Our decision rule is to contact the customer if the item pass and fail calibration when the results include the uncertainties and the customer must determine if the results meets their needs.


The calibration certificate shall not be reproduced except in full, without written approval of SP Metrology System (Thailand).

Calibrated by :



Calibration Officer

Approved by :

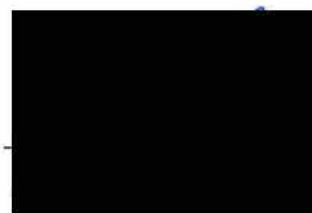

Authorized Signatory



ID LINE : IEC17025



Calibration Report

Certificate Number : SPR24060488-15

Page : 2 of 3

Reference Standards

Equipment Name	Model	Serial No.	Certificate No.	Due. Date
Sound Level Calibrator	ST-120	211203773	EEL.BP. 140/0167	26 Jan 2025

Traceability

This certification is traceable to the International System of Unit maintained at :

TISTR - Thailand Institute of Scientific and Technological Research



ID LINE : IEC17025



Result of Calibration

Certificate Number : SPR24060488-15

Page : 3 of 3

Range : 94 to 114 dB

Function : @1kHz

Select A

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.0	94.0	0.0	0.0	0.15
114	114.0	114.0	0.0	0.0	0.15

Select C

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.0	94.0	0.0	0.0	0.15
114	113.9	113.9	-0.1	-0.1	0.15

Note :

The result of calibration was found accurate as show on date and place of calibration only.
This Certificate is not certified for any commercial transaction.

Measurement Uncertainty

The reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor $k = 2.00$, providing a level of confidence approximately 95%.

- End of Certificate -



Page : 1 of 3

Customer : Life and Environment Co., Ltd.

90, 92, 94 Soi On-Nuch 64, Srinakarin Rd., On-Nuch, Suanluang,
Bangkok 10250

Equipment Name : Noise Dose Meter

Manufacturer : SOUNDTEK

Model : ST-130

Serial Number : 220100103

ID. Number : NT-06

Environmental Conditions

Ambient Temperature : $23^{\circ}\text{C} \pm 3^{\circ}\text{C}$

Received Date : 28 Jun 2024

Relative Humidity : 50 % \pm 15 %

Calibration Date : 28 Jun 2024

Location of Calibration : In-Lab

Recommend Due Date : 28 Jun 2025

Calibration Procedure : SP-CPE-04-01

Date of Issue : 29 Jun 2024

Method of Calibration

This certifies that the above instrument was calibrated in compliance with the calibration system requirement of ISO/IEC 17025:2017 in accordance with reference procedure. Standards used to perform this calibration are certified by to NIST or equivalent, National metrology institute, Natural physical constants, consensus standards. The result reported herein apply only to the calibration of the item described above as received. Our decision rule is to contact the customer if the item pass and fail calibration when the results include the uncertainties and the customer must determine if the results meets their needs.

The calibration certificate shall not be reproduced except in full, without written approval of SP Metrology System (Thailand).

Calibrated by :

Calibration Officer

Approved by :

Authorized Signatory



ID LINE : IEC17025



Calibration Report

Certificate Number : SPR24060488-14

Page : 2 of 3

Reference Standards

Equipment Name	Model	Serial No.	Certificate No.	Due. Date
Sound Level Calibrator	ST-120	211203773	EEL.BP. 140/0167	26 Jan 2025

Traceability

This certification is traceable to the International System of Unit maintained at :

TISTR - Thailand Institute of Scientific and Technological Research



ID LINE : IEC17025



Result of Calibration

Certificate Number : SPR24060488-14

Page : 3 of 3

Range : 94 to 114 dB

Function : @1kHz

Select A

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	93.4	93.4	-0.6	-0.6	0.15
114	113.3	113.3	-0.7	-0.7	0.15

Select C

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	93.3	93.3	-0.7	-0.7	0.15
114	113.2	113.2	-0.8	-0.8	0.15

Note :

The result of calibration was found accurate as show on date and place of calibration only.
This Certificate is not certified for any commercial transaction.

Measurement Uncertainty

The reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor $k = 2.00$, providing a level of confidence approximately 95%.

- End of Certificate -



ID LINE : IEC17025



Certificate of Calibration

Certificate Number : SPR24060488-16

Page : 1 of 3

Customer : Life and Environment Co., Ltd.

90, 92, 94 Soi On-Nuch 64, Srinakarin Rd., On-Nuch, Suanluang,
Bangkok 10250

Equipment Name : Noise Dose Meter

Manufacturer : SOUNDTEK

Model : ST-130

Serial Number : 220300020

ID. Number : NT-09

Environmental Conditions

Ambient Temperature : $23^{\circ}\text{C} \pm 3^{\circ}\text{C}$

Received Date : 28 Jun 2024

Relative Humidity : $50\% \pm 15\%$

Calibration Date : 28 Jun 2024

Location of Calibration : In-Lab

Recommend Due Date : 28 Jun 2025

Calibration Procedure : SP-CPE-04-01

Date of Issue : 29 Jun 2024

Method of Calibration

This certifies that the above instrument was calibrated in compliance with the calibration system requirement of ISO/IEC 17025:2017 in accordance with reference procedure. Standards used to perform this calibration are certified by to NIST or equivalent, National metrology institute, Natural physical constants, consensus standards. The result reported herein apply only to the calibration of the item described above as received. Our decision rule is to contact the customer if the item pass and fail calibration when the results include the uncertainties and the customer must determine if the results meets their needs.

The calibration certificate shall not be reproduced except in full, without written approval of SP Metrology System (Thailand).

Calibrated by :



Calibration Officer

Approved by :



Authorized Signatory



ID LINE : IEC17025



Calibration Report

Certificate Number : SPR24060488-16

Page : 2 of 3

Reference Standards

Equipment Name	Model	Serial No.	Certificate No.	Due. Date
Sound Level Calibrator	ST-120	211203773	EEL.BP. 140/0167	26 Jan 2025

Traceability

This certification is traceable to the International System of Unit maintained at :

TISTR - Thailand Institute of Scientific and Technological Research



ID LINE : IEC17025



Result of Calibration

Certificate Number : SPR24060488-16

Page : 3 of 3

Range : 94 to 114 dB

Function : @1kHz

Select A

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.0	94.0	0.0	0.0	0.15
114	113.7	113.7	-0.3	-0.3	0.15

Select C

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.0	94.0	0.0	0.0	0.15
114	113.8	113.8	-0.2	-0.2	0.15

Note:

The result of calibration was found accurate as show on date and place of calibration only.
This Certificate is not certified for any commercial transaction.

Measurement Uncertainty

The reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor $k = 2.00$, providing a level of confidence approximately 95%.

- End of Certificate -



ID LINE : IEC17025



Certificate of Calibration

Certificate Number : SPR24040397-3

Page : 1 of 3

Customer : Life and Environment Co., Ltd.

90, 92, 94 Soi On-Nuch 64, Srinakarin Rd., On-Nuch, Suanluang,
Bangkok 10250

Equipment Name : Noise Dose Meter

Manufacturer : SOUNDTEK

Model : ST-130

Serial Number : 170800296

ID. Number : NT-02

Environmental Conditions

Ambient Temperature : $23^{\circ}\text{C} \pm 3^{\circ}\text{C}$ Relative Humidity : $50\% \pm 15\%$

Location of Calibration : In-Lab

Calibration Procedure : SP-CPE-04-01

Received Date : 30 Apr 2024

Calibration Date : 04 May 2024

Recommend Due Date : 04 May 2025

Date of Issue : 05 May 2024

Method of Calibration

This certifies that the above instrument was calibrated in compliance with the calibration system requirement of ISO/IEC 17025:2017 in accordance with reference procedure. Standards used to perform this calibration are certified by to NIST or equivalent, National metrology institute, Natural physical constants, consensus standards. The result reported herein apply only to the calibration of the item described above as received. Our decision rule is to contact the customer if the item pass and fail calibration when the results include the uncertainties and the customer must determine if the results meets their needs.


The calibration certificate shall not be reproduced except in full, without written approval of SP Metrology System (Thailand).

Calibrated by :



Calibration Officer

Approved by :



Authorized Signatory



ID LINE : IEC17025



Calibration Report

Certificate Number : SPR24040397-3

Page : 2 of 3

Reference Standards

Equipment Name	Model	Serial No.	Certificate No.	Due. Date
Sound Level Calibrator	ST-120	211203773	EEL.BP. 140/0167	26 Jan 2025

Traceability

This certification is traceable to the International System of Unit maintained at :

TISTR - Thailand Institute of Scientific and Technological Research



ID LINE : IEC17025



Result of Calibration

Certificate No. : SPR24040397-3

Page : 3 of 3

Range : 94 to 114 dB

Function : @1kHz

Select A

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.0	94.0	0.0	0.0	0.15
114	114.0	114.0	0.0	0.0	0.15

Select C

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.0	94.0	0.0	0.0	0.15
114	113.9	113.9	-0.1	-0.1	0.15

Select Z

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.0	94.0	0.0	0.0	0.15
114	114.0	114.0	0.0	0.0	0.15

Note:

The result of calibration was found accurate as show on date and place of calibration only.
This Certificate is not certified for any commercial transaction.

Measurement Uncertainty

The reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor $k = 2.00$, providing a level of confidence approximately 95%.

- End of Certificate -



ID LINE : IEC17025



Certificate of Calibration

Certificate Number : SPR24040397-5

Page : 1 of 3

Customer : Life and Environment Co., Ltd.

90, 92, 94 Soi On-Nuch 64, Srinakarin Rd., On-Nuch, Suanluang,
Bangkok 10250

Equipment Name : Noise Dose Meter

Manufacturer : SOUNDTEK

Model : ST-130

Serial Number : 190500072

ID. Number : NT-05

Environmental Conditions

Ambient Temperature : $23^{\circ}\text{C} \pm 3^{\circ}\text{C}$

Received Date : 30 Apr 2024

Relative Humidity : $50\% \pm 15\%$

Calibration Date : 04 May 2024

Location of Calibration : In-Lab

Recommend Due Date : 04 May 2025

Calibration Procedure : SP-CPE-04-01

Date of Issue : 05 May 2024

Method of Calibration

This certifies that the above instrument was calibrated in compliance with the calibration system requirement of ISO/IEC 17025:2017 in accordance with reference procedure. Standards used to perform this calibration are certified by to NIST or equivalent, National metrology institute, Natural physical constants, consensus standards. The result reported herein apply only to the calibration of the item described above as received. Our decision rule is to contact the customer if the item pass and fail calibration when the results include the uncertainties and the customer must determine if the results meets their needs.


The calibration certificate shall not be reproduced except in full, without written approval of SP Metrology System (Thailand).

Calibrated by :



Calibration Officer

Approved by :

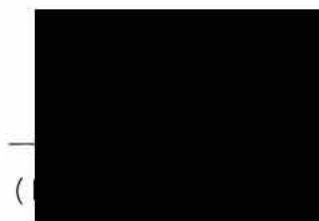

Authorized Signatory



ID LINE : IEC17025



Calibration Report

Certificate Number : SPR24040397-5

Page : 2 of 3

Reference Standards

Equipment Name	Model	Serial No.	Certificate No.	Due. Date
Sound Level Calibrator	ST-120	211203773	EEL.BP. 140/0167	26 Jan 2025

Traceability

This certification is traceable to the International System of Unit maintained at :
TISTR - Thailand Institute of Scientific and Technological Research



ID LINE : IEC17025



Result of Calibration

Certificate No. : SPR24040397-5

Page : 3 of 3

Range : 94 to 114 dB

Function : @1kHz

Select A

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.0	94.0	0.0	0.0	0.15
114	114.0	114.0	0.0	0.0	0.15

Select C

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.0	94.0	0.0	0.0	0.15
114	114.0	114.0	0.0	0.0	0.15

Select Z

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.0	94.0	0.0	0.0	0.15
114	113.9	113.9	-0.1	-0.1	0.15

Note:

The result of calibration was found accurate as show on date and place of calibration only.
This Certificate is not certified for any commercial transaction.

Measurement Uncertainty

The reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor $k = 2.00$, providing a level of confidence approximately 95%.

- End of Certificate -



Certificate of Calibration

Certificate Number : SPR24040397-4

Page : 1 of 3

Customer : Life and Environment Co., Ltd.

90, 92, 94 Soi On-Nuch 64, Srinakarin Rd., On-Nuch, Suanluang,
Bangkok 10250

Equipment Name : Noise Dose Meter

Manufacturer : SOUNDTEK

Model : ST-130

Serial Number : 190500065

ID. Number : NT-03

Environmental Conditions

Ambient Temperature : $23^{\circ}\text{C} \pm 3^{\circ}\text{C}$

Received Date : 30 Apr 2024

Relative Humidity : $50\% \pm 15\%$

Calibration Date : 04 May 2024

Location of Calibration : In-Lab

Recommend Due Date : 04 May 2025

Calibration Procedure : SP-CPE-04-01

Date of Issue : 05 May 2024

Method of Calibration

This certifies that the above instrument was calibrated in compliance with the calibration system requirement of ISO/IEC 17025:2017 in accordance with reference procedure. Standards used to perform this calibration are certified by to NIST or equivalent, National metrology institute, Natural physical constants, consensus standards. The result reported herein apply only to the calibration of the item described above as received. Our decision rule is to contact the customer if the item pass and fail calibration when the results include the uncertainties and the customer must determine if the results meets their needs.

The calibration certificate shall not be reproduced except in full, without written approval of SP Metrology System (Thailand).

Calibrated by :



Calibration Officer

Approved by :



Authorized Signatory



ID LINE : IEC17025



Calibration Report

Certificate Number : SPR24040397-4

Page : 2 of 3

Reference Standards

Equipment Name	Model	Serial No.	Certificate No.	Due. Date
Sound Level Calibrator	ST-120	211203773	EEL.BP. 140/0167	26 Jan 2025

Traceability

This certification is traceable to the International System of Unit maintained at :

TISTR - Thailand Institute of Scientific and Technological Research



ID LINE : IEC17025



Result of Calibration

Certificate No. : SPR24040397-4

Page : 3 of 3

Range : 94 to 114 dB

Function : @1kHz

Select A

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.0	94.0	0.0	0.0	0.15
114	114.0	114.0	0.0	0.0	0.15

Select C

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.0	94.0	0.0	0.0	0.15
114	113.9	113.9	-0.1	-0.1	0.15

Select Z

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.0	94.0	0.0	0.0	0.15
114	114.0	114.0	0.0	0.0	0.15

Note:

The result of calibration was found accurate as show on date and place of calibration only.
This Certificate is not certified for any commercial transaction.

Measurement Uncertainty

The reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor $k = 2.00$, providing a level of confidence approximately 95%.

- End of Certificate -

THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-67/0204

MTC No. EEL. BP. 117/0167

CALIBRATION CERTIFICATE

Submitted by : Life and Environment Co.,Ltd.

Address : 90, 92, 94 Soi On-Nuch 64, Srinakarin Rd., Suanluang, Bangkok, 10250.

Calibrated at : Electrical and Electronic Standards Laboratory, Industrial Metrology and Testing Service Centre.
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Rd., Muang, Samutprakan 10280.**Instrument Calibrated :**

Description : Acoustic Calibrator

Manufacturer : Quest Technologies

Model : QC-20

Serial No. : QOF110014

Ambient EnvironmentTemperature : $(23 \pm 3) ^\circ\text{C}$ Relative Humidity : $(50 \pm 15) \%$ Ambient Pressure : $(101.325 \pm 1.500) \text{ kPa}$

- Standards used :**
1. Digital Function Synthesizer NF Electronic DF-193A S/N 122037.
 2. Measuring Amplifier Bruel&Kjaer 2636 S/N 1537484.
 3. Programmable Attenuator Tamagawa TPA-303A S/N OF 2214.
 4. Digital Multimeter Agilent 34401A S/N MY44005560.
 5. Pressure Transmitter Vaisala PTB202AD S/N T0650001.
 6. Audio Analyzer Keithley 2015-P S/N 4106495.
 7. Condenser Microphone Bruel&Kjaer 4180 S/N 2889871.

Calibration Procedure: CP-102-04 based on IEC 60942-2003. The sound pressure level of instrument was measured by standard microphone using an insert voltage technique.

This instrument has been calibrated against standards maintained at Electrical and Electronic Standards Laboratory (EEL), which are traceable to the International System of Units through the National Institute of Metrology (Thailand).

The information on actual reading is attached herewith and the uncertainty limits quoted refer to the measured values only.

Date of Receipt : 12 Jan. 2024

Date of Calibration : 23 Jan. 2024

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.4

THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-67/0204

MTC No. EEL. BP. 117/0167

The reported expanded uncertainty is based upon a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%.

Nominal Output of Unit Under Test = 94 dB re 20 μ Pa at 1000 Hz

Acoustic Output in dB re 20 μ Pa, Corrected to Reference Conditions : 101.325 kPa, 23.0°C and 50 %RH

1. Sound Pressure Level

Standard Microphone Type	Measured Sound Pressure Level (dB)	Deviated value (dB)	Uncertainty (dB)	Tolerance limit IEC60942:2003 Class 1
1/2 inch Brüel&Kjaer 4180	93.96	-0.04	± 0.10	± 0.40 dB

2. Frequency

Standard Microphone Type	Measured Frequency (Hz)	Deviated value (Hz)	Uncertainty (Hz)	Tolerance limit IEC60942:2003 Class 1
1/2 inch Brüel&Kjaer 4180	999.3	-0.7	± 1.5	$\pm 1.0\%$

3. Total distortion

Standard Microphone Type	Measured Total distortion (%)	Uncertainty (%)	Tolerance limit IEC60942:2003 Class 1
1/2 inch Brüel&Kjaer 4180	2.65	± 0.60	$\pm 3.0\%$

Note : 1. No adjustment.

2. The calibrator pressure correction was not included.

3. The microphone volume correction was not included.

Date of Calibration : 23 Jan. 2024



The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.4

THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-67/0204

MTC No. EEL. BP. 117/0167

Nominal Output of Unit Under Test = 114 dB re 20 μ Pa at 1000 Hz

Acoustic Output in dB re 20 μ Pa , Corrected to Reference Conditions : 101.325 kPa , 23.0 °C and 50 %RH

1. Sound Pressure Level

Standard Microphone Type	Measured Sound Pressure Level (dB)	Deviated value (dB)	Uncertainty (dB)	Tolerance limit IEC60942:2003 Class 1
1/2 inch Bruel&Kjaer 4180	113.95	-0.05	± 0.10	± 0.40 dB

2. Frequency

Standard Microphone Type	Measured Frequency (Hz)	Deviated value (Hz)	Uncertainty (Hz)	Tolerance limit IEC60942:2003 Class 1
1/2 inch Bruel&Kjaer 4180	999.3	-0.7	± 1.5	$\pm 1.0\%$

3. Total Distortion

Standard Microphone Type	Measured Total Distortion (%)	Uncertainty (%)	Tolerance limit IEC60942:2003 Class 1
1/2 inch Bruel&Kjaer 4180	0.35	± 0.50	$\pm 3.0\%$

Note : 1. No adjustment.

2. The calibrator pressure correction was not included.

3. The microphone volume correction was not included.

Calibrated by :



Approved by :



Director

Electrical and Electronic Standards Laboratory

Industrial Metrology and Testing Service Centre

Date of Calibration : 23 Jan. 2024

Date of Issue : 24 Jan. 2024

Ref : 2011267011200168001

End of Certificate

3 / 3

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.4

Accredited by

NSC-TISI-TIS 17025

Calibration 0426



Calibration certificate

Calibration Certificate No. 23BCI0349

Object	Electronic non-automatic weighing instrument	This calibration certificate documents the traceability to national standards.
Manufacturer	Sartorius	Uncertainties of measurements are taken into account when only statements of compliance are made.
Type	MSE125P-100-DU	This certificate was prepared by Sartorius Corporation in accordance to the current ISO/IEC 17025:2017 standard and Sartorius Work Instruction (Method) SOP WI 08.
Serial QM Ident. no.	0028606077 N/A	This certificate relate and apply this equipment only.
Customer	Life and Environment Co., Ltd.	
	90, 92, 94 Soi On-Nuch 64, Srinakarin Road, On-Nuch, Suanluang, Bangkok 10250. Thailand.	
Order no.	218684	
Number of pages	4	
Date of calibration	15 Sep 2023	

This calibration certificate may not be reproduced other than in full except with the permission of NSC-TISI-TIS-17025 and the issuing laboratory. Calibration certificates without signature are not valid.

The user is obliged to have the object recalibrated at appropriate intervals.

Date	15 Sep 2023	Approval of the Calibration Certificate	Person in charge
			

Calibration object

Multi interval instrument

Model	MSE125P-100-DU	
Serial Number	0028606077	
QM Ident. no Inventory no.	N/A —	
Range	1	2
Maximum capacity (Max. load)	60.00000 g	120.0000 g
Measured range	60.00000 g	120.0000 g
Scale interval	0.00001 g	0.0001 g

Place of calibration

Address	According to page 1
Department Cost center	Laboratory Testing. —
Building Floor	— 1st Floor.
Room	Air(TSP/PM10) Testing Laboratory.
Maximum temperature variation at place of calibration	5 K

Calibration procedure

EURAMET cg-18, V4.0 - Guidelines on the Calibration of Non-Automatic Weighing Instruments

Test equipment

Test equipment type	Test equipment ID	Valid until
Thermometer	MHB382-SD Cer No.C19231845,(Traceable to SI unit through DKSH)	23 Aug 2024
Test weight set OIML R111 E2	Certificate No.M2308197S ,E2(Traceable to SI unit through TCS)	23 Aug 2026

Adjustment Status

The measuring device was internally adjusted before the calibration.

Environmental and measuring conditions

Date of calibration 15 Sep 2023

Temperature at place of calibration | Temp. diff.
T_{weights} - T_{place} 25.8 °C | 0.2 K

Measuring conditions The installation site is suitable. The device was levelled. Balance was loaded up to Max before test.

Comments Humidity 40.0 %RH.

Measurement results | Measurement uncertainties

Repeatability

Test load (nominal): 50 g | 100 g

	50 g	100 g
1	50.00002 g	100.0000 g
2	50.00001 g	100.0000 g
3	50.00001 g	100.0000 g
4	50.00001 g	100.0000 g
5	50.00001 g	100.0000 g
6	50.00002 g	100.0000 g
7	50.00002 g	99.9999 g
8	50.00002 g	100.0000 g
9	50.00001 g	100.0000 g
10	50.00002 g	100.0000 g
	s = 0.000005 g	s = 0.00003 g

Eccentricity

Test load (nominal):	50 g
Center	50.00002 g
Front left	50.00001 g
Back left	50.00004 g
Back right	50.00004 g
Front right	50.00001 g
Maximum deviation from centric loading indication Δ/ecc max = 0.00002 g	

Error of indication

Testload	Indication	Error	Expansion factor	Uncertainty	Uncertainty relative
L	I	E	k	U(E)	U _{rel} (E)
0.01000 g	0.01000 g	0.00000 g	2.00	0.000024 g	-0.24 %
0.10000 g	0.10000 g	0.00000 g	2.00	0.000037 g	0.037 %
1.00000 g	1.00000 g	0.00000 g	2.00	0.000037 g	0.0037 %
10.00002 g	10.00002 g	0.00000 g	2.00	0.000069 g	0.00069 %
20.00002 g	20.00002 g	0.00000 g	2.00	0.000069 g	0.00034 %
55.00004 g	55.00003 g	-0.00001 g	2.00	0.00017 g	0.00031 %
70.0000 g	70.0000 g	0.0000 g	2.00	0.00017 g	0.00024 %
80.0001 g	80.0001 g	0.0000 g	2.00	0.00018 g	0.00023 %
100.0000 g	100.0000 g	0.0000 g	2.00	0.00017 g	0.00017 %
110.0000 g	110.0000 g	0.0000 g	2.00	0.00028 g	0.00025 %
120.0000 g	120.0000 g	0.0000 g	2.00	0.00028 g	0.00023 %

Maximum error of indication |E|_{max} = 0.00001 g

U_{rel}(E) is the quotient of U(E) and test load L. The uncertainty of measurement U(E) is valid only if error E is considered. You will find reference notes on the uncertainty of measurement in use under: Appendix to the calibration certificate | Interpretation of measurement results.

Reference note: The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the documented Expansion factor, determined in accordance with the European Calibration Guideline EURAMET cg-18, V4.0. There is a 95 % probability that the value of the measurand will be in the assigned value range.

End of calibration certificate

Uncertainty of measurement in use

Device adjusted before measurement

Yes

Temperature deviation considered

1.5 K (isoCAL active)

Temperature coefficient considered

$1 \cdot 10^{-6}/K$

Uncertainty of the weighing result $U_{gl}(W)$

Partial weighing range 1 | 0.00000 g...60.00000 g

$U_{gl}(W) = 0.000013 \text{ g} + 3.20 \cdot 10^{-6} \cdot R$


Partial weighing range 2 | 60.00000 g...120.0000 g

$U_{gl}(W) = 0.000086 \text{ g} + 2.77 \cdot 10^{-6} \cdot R$

Reference note: The current uncertainty of measurement is calculated by entering of the reading R into this formula. In relation to this, there is no need for a correction of the indication error. The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied with an Expansion factor of 2, determined in accordance with the European Calibration Guideline EURAMET cg-18, V4.0. There is a 95 % probability that the value of the measurand will be in the assigned value range.

Indication in % from Max1	Net indication R	Uncertainty $U_{gl}(W)$	Uncertainty relative $U_{gl}(W)_{rel}$
1 %	0.60000 g	0.000015 g	0.0025 %
25 %	15.00000 g	0.000061 g	0.00041 %
50 %	30.00000 g	0.00011 g	0.00036 %
75 %	45.00000 g	0.00016 g	0.00035 %
100 %	60.00000 g	0.00021 g	0.00034 %

Graphic realization of the relative uncertainty of measurement | process accuracy

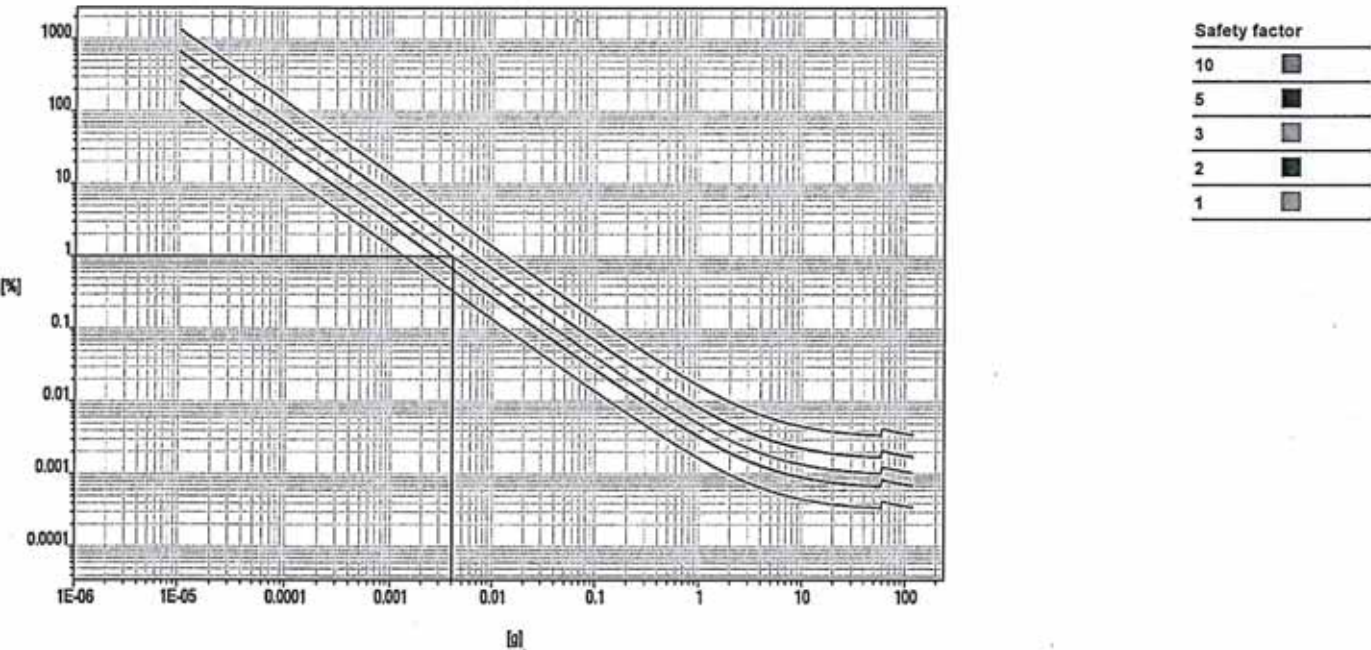

Displayed example

Process accuracy

1.00 %

Safety factor

3

Minimum sample weight

0.00400 g

UUT Meter Console Information

Model #:	XC-572
Serial #:	605186
DGM Model #:	SK25EX
DCM Serial #:	0005288

Calibration Conditions

Bar. Pressure (mm Hg):	756.0
Ambient Temperature (°C):	25.7
Relative Humidity (%):	65
Altitude (m):	1.50
Bar. Pressure Corr. (mm Hg):	755.9

Calibration Reference

Work No.:	SVO26796
Calibration No.:	SA2023001
Serial No.:	546321
Cal.Due	24-Mar-24
Serial No.:	9038005

Judgment : **Pass** According to note :

Factors/Conversions

Std. Temp. (K):	298.15
Std. Press. (mm Hg):	760
K ₁ (K/mm Hg):	0.3923

UUT Meter (DGM)

Run Time (seconds)	Orifice, ΔH (mm H ₂ O)	Volume		Meter Temperature (°C)		Meter Pressure (mm H ₂ O)	Reference Meter (WTM)		Outlet Temperature (°C)	
		Initial (L)	Final (L)	Initial	Final		Initial	Final	Initial	Final
Θ	P _{m(g)}	V _{m(l)}	V _{m(l)}	t _{m(l)}	t _{m(l)}	P _w	V _{w(l)}	V _{w(l)}	t _{w(l)}	t _{w(l)}
900	13.00	512699.1	512869.5	28.0	28.0	-1.0	431236.86	431410.21	26.5	26.5
600	25.00	511923.9	512081.6	28.0	28.0	-1.0	430461.99	430622.64	26.5	26.5
480	50.00	512090.4	512268.0	28.0	28.0	-1.0	430633.55	430815.39	26.5	26.5
420	80.00	512282.1	512480.5	28.0	28.0	-1.0	430825.43	431026.44	26.5	26.5
300	120.00	512512.2	512681.9	28.0	28.0	-1.0	431052.74	431225.49	26.5	26.5

Standardized Data

Reference Meter (L)		UUT Meter (L)		Correction Factor		ΔH @ (mm H ₂ O)	
Std. Vol.	Std. Flow	Std. Vol.	Std. Flow	Value	Variance	ΔH@	ΔH@
V _{w(Std)}	Q _{w(Std)}	V _{m(Std)}	V _{w(Std)}	Y	ΔY	ΔH@	ΔH@
170.71	11.38	168.00	11.4	1.0161	0.0035	45.0	-0.368
158.20	15.82	155.66	15.8	1.0164	0.0037	44.8	-0.532
179.07	22.38	175.73	22.4	1.0190	0.0064	44.9	-0.466
197.95	28.28	196.88	28.3	1.0054	-0.0072	45.1	-0.223
170.12	34.02	169.05	34.0	1.0063	-0.0063	46.9	1.589
				= Y Avg.		= ΔH@ Avg. (Metric)	
				1.0127		45.3	

Note1 : For Calibration Factor Y, the ratio of the reading of the calibration meter to the dry gas meter, acceptable tolerance of individual values from the average is ±0.02.

Note2 : For ΔH_g, orifice pressure differential that equates to 0.0212m³/min at standard temperature and pressure, acceptable tolerance of individual values from the average is ±0.2inches (5.1mm) H₂O.

Calibrator :

Signature :

Date : 28/Nov/23

The instruments listed and described on this certificate have been calibrated against standards traceable to the National Institute of Standards and Technology (NIST) and in reference to EPA Method 5, Section 10.3.1.

Calibration Certificate Appendix

METHOD 5 PRE-TEST CONSOLE CALIBRATION

Calibration No.: **SA2023001**

<p>UUT Meter / Console Information</p> <p>Model #: <u>XC 572-V</u> Serial number: <u>605186</u> DGM Model #: <u>SK25EX</u> Serial number: <u>0005288</u></p> <p>Check the Diagnosis Check the system before calibrating.</p> <table style="width: 100%;"> <tr> <td style="width: 50%;"> <input type="checkbox"/> Visual instrument normalcy <input type="checkbox"/> Electrical and Temperature Systems <input type="checkbox"/> Inclined Manometer with Systems <input type="checkbox"/> Pressure Gauge <input type="checkbox"/> Leak Check <input type="checkbox"/> PM and Calibration </td> <td style="width: 50%;"> <input type="checkbox"/> Vacuum: Pass <input checked="" type="checkbox"/> Pressure: Pass <input type="checkbox"/> Repairing before Calibration </td> </tr> <tr> <td style="width: 50%;"> <input type="checkbox"/> Not Passed </td> <td style="width: 50%;"> <input checked="" type="checkbox"/> Passed </td> </tr> </table>	<input type="checkbox"/> Visual instrument normalcy <input type="checkbox"/> Electrical and Temperature Systems <input type="checkbox"/> Inclined Manometer with Systems <input type="checkbox"/> Pressure Gauge <input type="checkbox"/> Leak Check <input type="checkbox"/> PM and Calibration	<input type="checkbox"/> Vacuum: Pass <input checked="" type="checkbox"/> Pressure: Pass <input type="checkbox"/> Repairing before Calibration	<input type="checkbox"/> Not Passed	<input checked="" type="checkbox"/> Passed	<p>Nomenclature</p> <p>Pb - Barometric Pressure DGM - Dry Gas Meter K₁ - Constant based on standard temp and press Θ - Run time, in minutes P_m - ΔH (Meter Pressure, gauge) V_m - Volume collected by test meter, corrected for STP Q_{m(std)} - Calculated flow rate of test meter K' - Critical orifice coefficient P_{ref} - Measured pressure of reference meter T_{ref} - Temperature measured in reference meter T_m - Temperature measured in test meter Y - Ratio of volume collected from test meter and orifice</p>
<input type="checkbox"/> Visual instrument normalcy <input type="checkbox"/> Electrical and Temperature Systems <input type="checkbox"/> Inclined Manometer with Systems <input type="checkbox"/> Pressure Gauge <input type="checkbox"/> Leak Check <input type="checkbox"/> PM and Calibration	<input type="checkbox"/> Vacuum: Pass <input checked="" type="checkbox"/> Pressure: Pass <input type="checkbox"/> Repairing before Calibration				
<input type="checkbox"/> Not Passed	<input checked="" type="checkbox"/> Passed				

Equations

$$K_1 = \frac{T_{std}}{P_{std}}$$

$$V_{w(std)} = Y * K_1 \frac{V_w * (P_{bar} + \frac{P_{w(std)}}{13.6})}{T_m}$$



$$V_{m(std)} = \frac{K_1 V_m (P_{bar} + \frac{P_{w(std)}}{13.6})}{T_m}$$

$$Y = \frac{V_{w(std)}}{V_{m(std)}}$$

$$Q_{w(std)} = \frac{V_{w(std)}}{\Theta}$$

$$Metric \Delta H_0 = \frac{P_{m(g)} * 0.001036 * (P_{bar} + \frac{P_{w(std)}}{13.6})}{T_m} * \left(\frac{T_v * \Theta}{V_v * P_{bar}} \right)^2$$

Calibration Graphs

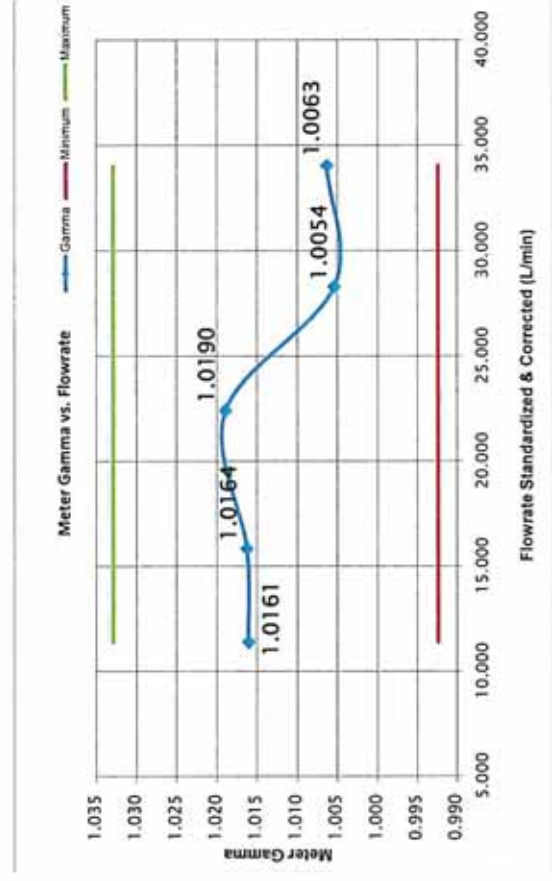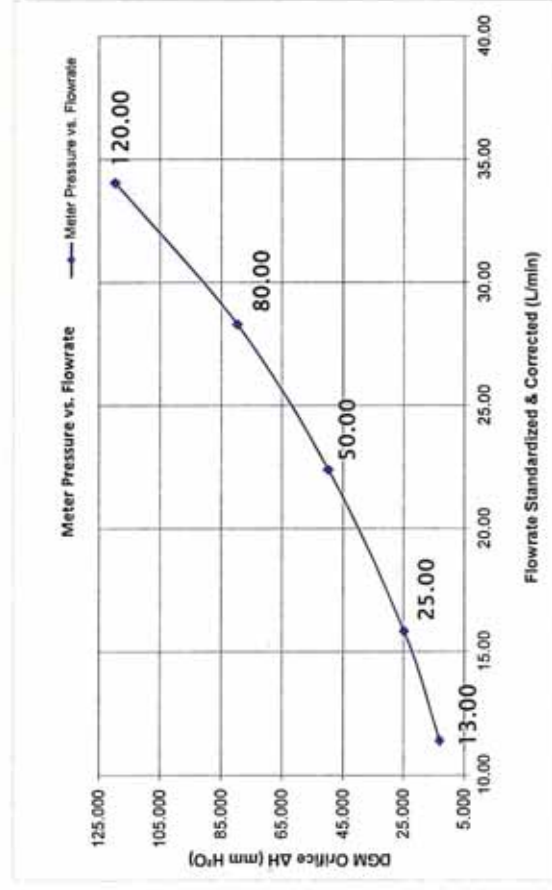

Certificate of Calibration

Method 5 Console Sensor Calibration - Metric Units

page: 1/1

Console Information

Model #: XC-572
Serial #: 605186
Units: Metric

Calibration Conditions

Pbar (mm. Hg): 759.60
Humidity (%): 65
Tamb (°C): 25.6
Elevation (m): 1.5
Corr. Pbar (mm. Hg): 759.60

Calibration Reference

Calibration No.: SA2023001
Work No.: SVO26796

Reference Devices

TC Calibrator Model: FLUKE 714
Serial No.: 9038005

Temperature Sensors Calibration Data

Reference Temp.		Test Thermocouple Calibrations						Reference Point Status ²
		Aux	Stack	Probe	Oven	Filter	Exit	
Point	°C	°C	°C	°C	°C	°C	°C	Pass/Fail
1	-18	-17	-17	-17		-17	-17	PASS
2	38	38	38	38		39	39	PASS
3	93	94	94	94		95	94	PASS
4	149	151	151	150		150	150	PASS
5	260	261	261	261		261		PASS
6	371		374					PASS
7	482		486					PASS
8	593		597					PASS
9	816		824					PASS
10	1038		1046					PASS
		±3.0°C, 5.4°F	1.50%	±3.0°C, 5.4°F	±3.0°C, 5.4°F	±3.0°C, 5.4°F	±1.0°C, 2.0°F	PASS

Overall Audit Status

DGM Temperature Sensor

Ref Point	Reference Temp.	DGM Thermocouple Sensor Reading	Δt_{abs}	Maximum	Reference Status ² (±1%)
#	°C	°C	°C	%	Pass/Fail
Ice Water	0.2	0	0.07%	0.08%	PASS
Ambient	25.6	26	0.08%		

Temperature Controller

Heater Controller	Reference Measure	XC-572	Deviated to set point	ΔT_{abs} ±3%	Temp. Controller Status ³
Set point	(μ)	Thermometer	°C	°C	Pass/Fail
120 °C	°C	°C	°C	°C	PASS
Probe	123	125	-2	0.50%	PASS
Filters	120	121	-1	0.25%	PASS
Heated Box	120	119	1	0.25%	PASS

Notes
¹ Suggested, minimum reference points are 10 (0, 100, 200, 300, 500, 700, 900, 1100, 1500, 1900 °F), can test for more.

² For valid test results, the maximum difference between test and reference readings should be temperature from the reference reading and the exit thermocouple which should be less than 2°F (1 °C) from the reference reading (EPA Method 2, Section 6.3 and EPA Method 5, Sections 6.1.1.7-6.1.1.8)

³ Heater control acceptance limit Temperature can be maintained at 120 °C ±14 °C, ±57 °F within ±1.5%⁽²⁾ at a flow rate of 20 lpm.

Signature:

Date: 28/Nov/23

I certify that the above Thermocouple Sensors were calibrated in accordance with US EPA Methods 2 and 5, CFR 40 Part 60.

Console Sensor Audit QA Sheet

Meter Console Information (UUT)

Model #: XC-572
Serial #: 605186
Units: Metric

Calibration Conditions

Pbar (mm. Hg): 30.00
Humidity (%): 65%
Amb. Temp. (°C): 69
Altitude (m): 100.0
Corrected Pbar (mm. Hg): 29.90

Calibration No. : SA2023001

Work No. : SVO26796

Reference Devices

TC Calibrator Model: FLUKE 714
Serial No.: 9038005
Digital Manometer Model: Dwyer DPGA-00
Serial No.: 721

Audit Data

Reference Point	Reference Temp.	Console Thermocouple Audit						Reference Point Status ¹
		Aux	Stack	Probe	Oven	Filter	Exit	
#	°C	°C	°C	°C	°C	°C	°C	Pass/Fail
1	26.5	27	27	27	27	27	27	PASS
Acceptance criteria		3.0°C, 5.4°F	1.50%	3.0°C, 5.4°F			1.0°C, 2.0°F	

Reference Thermocouple ID: 90728323

Ref Point	Reference Temp.	DGM Thermocouple Sensor Reading	ΔTabs4	Maximum	Reference Status (±1%)
#	°C	°C	°C	%	Pass/Fail
Ice Water	0.2	0	0.07%	0.08%	PASS
Ambient	25.6	26	0.08%		

Internal temperature thermocouple is not audited to EPA standards, and should not be used as an official reference for ambient temperature.

Console Vacuum Audit			
Reference Point	Reference Vacuum	Console Vacuum	Reference Point Status ³
#	mm. Hg	mm. Hg	Pass/Fail
1	23.90	24.00	PASS

Notes

¹For valid test results, the maximum difference between test and reference readings should be temperature from the reference reading and the exit thermocouple which should be less than 2°F (1 °C) from the reference reading (EPA Method 2, Section 6.3 and EPA Method 5, Sections 6.1.1.7-6.1.1.8)

²For valid test results, the maximum difference between console and reference vacuum readings should be less than 0.5 in. Hg (12.5 mmHg)

Signature: _____

Date: 28/Nov/23

I certify that the above Thermocouple, Barometric, and Vacuum Sensors were calibrated and audited in accordance with US EPA Methods, CFR 40 Part 60.

Nozzle Calibration

Nozzle Information

Manufacturer Apex
Type Stainless Steel
Identification -

Calibration Conditions

Bar. Pressure (mm Hg): 756.5
Ambient Temperature (°C): 26.0
Relative Humidity (%): 65

Calibration Reference

Calibration No.: SA2023001
SITHIPORN
Work No.: SVO26796
Units: Metric

Reference Equipment

Vernier, 0-250mm 0.01 mm increments model Mitutoyo

Serial No

3038570

Cal No.:

L202310355-0001

Cal.due:

07/Nov/23

Calibration Method

Follow the USEPA Method 5 nozzle size calibration procedure. (ref. 40 CFR PART 60).

Calibration Result


ID No.	Sizes	measured every 60° nozzle			(D ₁ + D ₂ + D ₃) / 3	Different ≤ 0.100 mm.	
	mm.	D ₁	D ₂	D ₃	Davg	1	Judgment
4	3.1	3.18	3.17	3.17	3.173	0.010	PASS
6	4.6	4.42	4.44	4.46	4.440	0.040	PASS
8	6.2	6.22	6.19	6.23	6.213	0.040	PASS
10	7.8	7.78	7.78	7.77	7.777	0.010	PASS
12	9.4	9.37	9.39	9.40	9.387	0.030	PASS
14	10.9	10.85	10.87	10.87	10.863	0.020	PASS
16	12.6	12.74	12.75	12.78	12.757	0.040	PASS

Where :

D₁, D₂, D₃ = There difference nozzle diameters at 60 degrees to each other,
each measured to the nearest 0.025 mm or 0.001 inch

Δ D = Maximum difference between any two diameters, must be ≤ 0.100 mm or 0.004 inch

D avg = (D₁ + D₂ + D₃) / 3



Signature

Date : 28/Nov/23

Sampling Probe and Pitot validation

Sampling Probe Information

Manufacturer: Apex
Probe Type: SS, 6ft
Probe No.: -
Pitot tube Type: S Type 3/8 Inc.
Pitot tube No.: -

Calibration Conditions

Bar. Pressure (mm Hg): 759.5
Ambient Temperature (°C): 26.0
Relative Humidity (%): 53
Units: Metric

Calibration Reference

Calibration No.: SA2023001
Work No.: SVO26796


Reference Devices

- Vernier, 0-250mm 0.01 mm increments
Model: Mitutoyo, ID No.: EPD1-VER-57-1-CEN-01

Validation method : Follow the USEPA Method 5 pitot tubes (S type) calibration procedure. (ref. 40 CFR PART 60).

Sampling Probe Validation with Tune up





☑ : Measuring and aligning with 1/2" sample nozzle(12.7 mm)

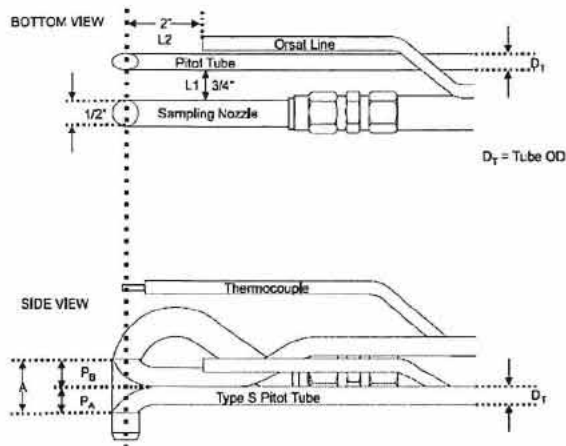

Measured	Acceptance Standard
$L_1 = 18.56 \text{ mm}$	(19.05 mm. or 0.75 in.)
$L_2 = 47.69 \text{ mm}$	(50.8 mm. or 2.0 in.)
$D_T = 9.52 \text{ mm}$	(9.525 mm., 0.375 in.)
$A = 22.07 \text{ mm}$	($2.1 D_T \leq A \leq 3D_T$)
$A/2D_T = 1.159 \text{ mm}$	($1.05 P_A / D_T \leq A \leq 1.5$)

Pitot Tube Validations and Engles measurement Result

☑ : Measure results after maintenance and adjustments.

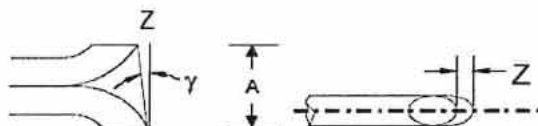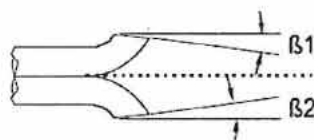

P_B Size	Acceptance of correctness
$\alpha_1 = 0.55^\circ$	$\leq 10^\circ$
$\beta_1 = 2.15^\circ$	$\leq 5^\circ$
P_A Size	
$\alpha_2 = 0.65^\circ$	$\leq 10^\circ$
$\beta_2 = 1.90^\circ$	$\leq 5^\circ$

Engles measurement

	Calculated Result	Acceptance Criteria
$W = 0.80^\circ$	0.318 mm	$W < 0.0794 \text{ mm. (0.03125 in)}$
$Z = 0.30^\circ$	0.116 mm	$Z < 3.175 \text{ mm. (0.125 in.)}$

Can be use 0.84 for $C_p(s)$ if the type of face-opening misalignmnet show above with not affect the base line value of $C_p(s)$
Solong as standard range.

Signature: _____

Date: 28/Nov/23

Certificate of Calibration

DGM with Totalizer Calibration - Liters (L)

UUT Meter Console Information

Model :	XC-572
Serial :	605186
Totalizer display:	N/A
DGM model :	SK25EX
Serial :	0005288

Calibration Conditions

Bar. Pressure (mm Hg):	755.0
Ambient Temperature (°C):	25.7
Relative Humidity (%):	65
Altitude (m):	1.50

Factors/Conversions

Std. Temp. (K):	298.15
Std. Press. (mm Hg):	760
K ₁ (K/mm Hg):	0.3923

Work No.: SVO26769

Calibration No.: SA2023001

Reference Equipment

WTM Model:	W-NK-5A	WTM Serial:	535476
WTM Cal. Due Date:	25-Mar-23	Gamma:	0.9976
Thermometer:	Fluke 714	Serial #:	N/A

UUT Meter (DGM)

Run Time (seconds)	Flow Rate (Rotameter)	Volume(L)			Meter Temperature (°C)		Meter Pressure (mm H ₂ O)	Volume (L)			Outlet Temperature (°C)	
		Initial	Final	Total	Initial	Final		Initial	Final	Total	Initial	Final
Θ	(L/Min)	V _{wi}	V _{wf}	V _w	t _{mi}	t _{mf}	P _w	V _{wi}	V _{wf}	V _w	t _{wi}	t _{wf}
900	1.00	514431.90	514445.70	13.80	27.0	27.0	-1.0	433294.69	433308.92	14.23	27.0	27.0
600	2.00	514399.70	514419.40	19.70	27.0	27.0	-1.0	433262.98	433283.21	20.23	27.0	27.0
480	2.50	514488.80	514508.20	19.40	27.0	27.0	-1.0	433352.74	433372.69	19.95	27.0	27.0
420	3.00	514354.30	514375.50	21.20	27.0	27.0	-1.0	433214.91	433236.63	21.72	27.0	27.0
300	4.00	514285.50	514305.70	20.20	27.0	27.0	-1.0	433129.27	433149.95	20.68	27.0	27.0

Standardized Data

Scaling Factor

Test meter		Reference Meter		Gamma		Rotameter Calibration	
Std. Vol.	Std. Flow Rate	Std. Volume	Std. Flow Rate	Value	Variation	Rotameter	Std. Flow.
V _{mstd} (L)	Q _{wstd} (L/min)	V _{wstd} (L)	Q _{wstd} (L/min)	Y	ΔY	(L/Min)	(L/min)
13.637	0.935	14.026	0.935	1.0285	0.004	1.00	0.94
19.470	1.994	19.940	1.994	1.0241	0.000	2.00	1.99
19.174	2.458	19.664	2.458	1.0255	0.001	2.50	2.46
20.954	3.058	21.408	3.058	1.0217	-0.002	3.00	3.06
19.968	4.077	20.383	4.077	1.0208	-0.003	4.00	4.08
				1.0241	DGM Y Avg.⁽¹⁾		

Note:1. For Calibration Factor Y, the ratio of the reading of the calibration meter to the dry gas meter, acceptable tolerance of individual values from the average is ± 0.02 .

Note:2. For the Scaling Calibration Factor (SC), it is the ratio of the display to adjust the Y value to be close to 1.000, equal to the reference standard.

Technical:

Signature:

Date:

28/Nov/2023

The instruments listed and described on this certificate have been calibrated against standards traceable to the National Institute of Standards and Technology (N.I.S.T.) and in reference to EPA Method 5, Section 10.3.1. and EPA Method 6, Section 10.1.3.

Sithiporn Associate Co., Ltd Environmental / Hygiene Department (ENV) Web site : www.sithiporn.com # E-mail: service2-env@sithiporn.com



Revised: 2023/01/23

Calibration Certificate Appendix

DGM with Totalizer Calibration

Nomenclature	Equations
<p>P_b - Barometric Pressure</p> <p>DGM - Dry Gas Meter</p> <p>K_1 - Constant based on standard temp and press</p> <p>Θ - Run time, in minutes</p> <p>$P_m - \Delta H$ (Meter Pressure, gauge)</p> <p>V_m - Volume collected by test meter, corrected for STP</p> <p>$Q_{m(std)}$ - Calculated flow rate of test meter</p> <p>K' - Critical orifice coefficient</p> <p>P_w - Measured pressure of reference meter</p> <p>t_w - Temperature measured in reference meter</p> <p>t_m - Temperature measured in test meter</p> <p>Y - Ratio of volume collected from test meter and orifice</p> <p>sc - Scaling Factor</p> <p>Counts_{std} - Number of pulse counts, standardized</p> <p>C_{raw} - Number of raw pulse counts of a calibration run</p>	$V_{w(std)} = Y * K_1 \frac{V_w * (P_{bar} + \frac{P_{m(g)}}{13.6})}{T_w}$ $V_{m(std)} = Counts_{std} * Y_{sc(avg)}$ $Counts_{std} = K_1 \frac{C_{total} * (P_{bar} + \frac{P_{m(g)}}{13.6})}{T_m}$ $K_1 = \frac{T_{std}}{P_{std}}$ $Q_{w(std)} = \frac{V_{w(std)}}{\Theta}$ $Y_{sc} = \frac{V_{w(std)}}{Counts_{std}}$ $Y = \frac{V_{cr(std)}}{V_{m(std)}}$

Calibration Graphs

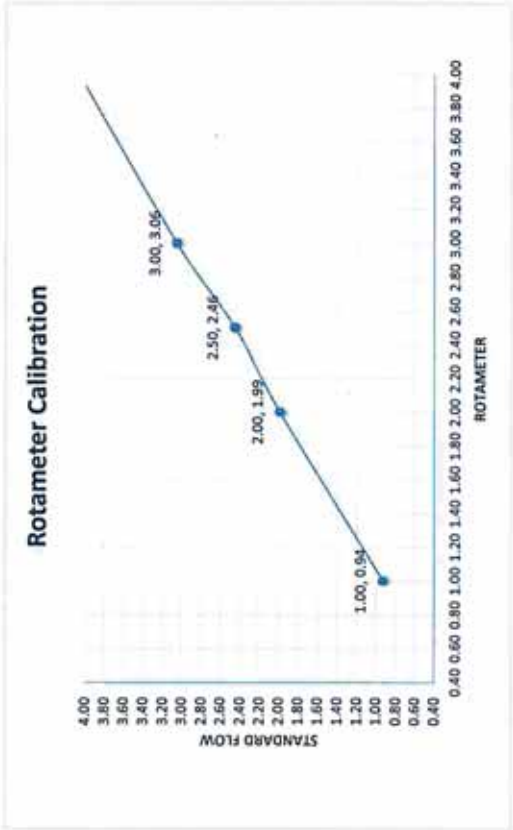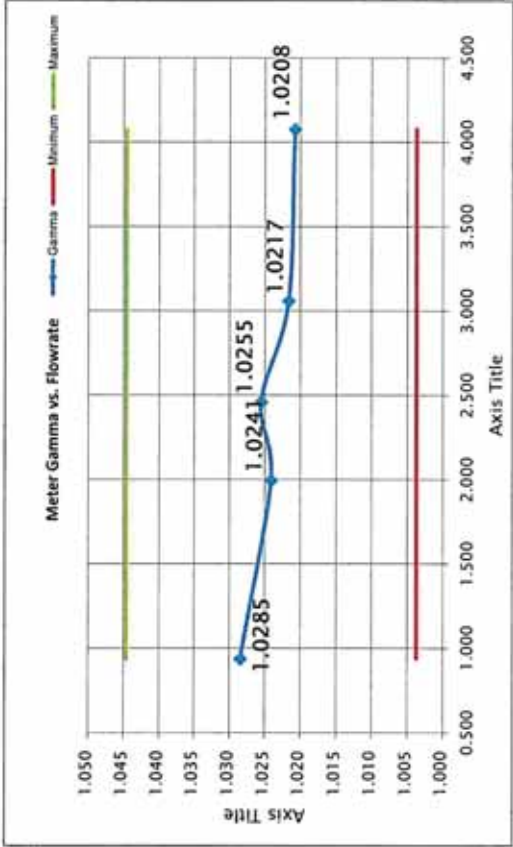

Certificate of Calibration

Method 6 Console Sensor Calibration - Metric Units

page: 1/1

Console Information

Model #:	XC-572
Serial #:	605186
Temp Dsp:	LASCAR
Serial :	DTM-995B
Units:	Metric

Calibration Conditions

Pbar (mm. Hg):	759.40
Humidity (%):	47
Tamb (°C):	24.44
Elevation (m):	1.5
Corr. Pbar (mm. Hg):	759.4

Calibration Reference

Calibration No. :	SA2023001
Work No. :	SVO26769
Reference Devices	
TC Calibrator Model:	FLUKE 714
Serial No.:	9038005

Temperature Sensors Calibration Data

Reference Temp.		Test Thermocouple Calibrations					Reference Point Status ²
		Aux	Stack	Probe	Filter	Exit	
Point	°C	°C	°C	°C	°C	°C	Pass/Fail
1	-18	-18	-18	-18	-18	-18	PASS
2	38	39	39	39	39	39	PASS
3	93	95	95	95	95		PASS
4	149	150	150	150	150		PASS
5	260	261	262	262	262		PASS
6	371		374				PASS
7	482		484				PASS
8	593		597				PASS
9	816		823				PASS
10	1038		1049				PASS
		±3.0°C, 5.4°F	1.50%	±3.0°C, 5.4°F	±3.0°C, 5.4°F	±2.0°C, 3.6°F	PASS

Overall Audit Status

DGM Temperature Sensor

Ref Point	Reference Temp.	DGM Thermocouple Sensor Reading	Δt_{abs}	Maximum	Reference Status ² (±1%)
#	°C	°C	°C	%	Pass/Fail
Ice Water	0.2	0	0.07%	0.45%	PASS
Ambient	25.6	28	0.45%		

Temperature Controller

Heater Controller	Reference Measure	XC-572	Deviated to	ΔT_{abs}	Temp. Controller Status ³
Set point	(μ)	Thermometer	set point	±3%	
120 °C	°C	°C	°C	°C	Pass/Fail
Probe	123	125	-2	0.50%	PASS
Filters	120	121	-1	0.50%	PASS

Notes

¹ Suggested, minimum reference points are 10 (0, 100, 200, 300, 500, 700, 900, 1100, 1500, 1900 °F), can test for more.

² For valid test results, the maximum difference between test and reference readings should be temperature from the reference reading and the exit thermocouple which should be less than 2°F (1 °C) from the reference reading (EPA Method 2, Section 6.3 and EPA Method 5, Sections 6.1.1, 7-6.1.1.8)

³ Heater control acceptance limit Temperature can be maintained at 120 °C ±14 °C, ±57 °F within ±1.5%⁽²⁾ at a flow rate of 20 lpm.

Signature: _____

Date : 28/Nov/23



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG, BANGKOK 10250
TEL. 0-2717-3000-24 FAX. 0-2719-9484



Certificate of Calibration

Certificate No. : 24P202

Page : 1 of 2

Equipment : Digital Manometer

Manufacturer: Dwyer

Model : 477

Serial No.: 477-5-FM

ID No.: SP-362

Condition As-Received: Used Item

Received Date: 09 January 2024

Calibration Date: 17 January 2024

Reference: 2401-0234WN

Submitted by: LIFE & ENVIRONMENT CO., LTD.

Ambient Temperature: (23 ± 2) °C

Relative Humidity: (50 ± 15) %

Atmospheric Pressure: 1014 mbar

This certificate may not be reproduced other than in full,
except with the prior written approval of the head of
Corporate Services 3: Equipment Calibration and Testing Services.

90, 92, 94 Soi On-Nuch 64, Srinakarin Road,
On-Nuch, Suanluang, Bangkok 10250

Procedure used: The calibration was conducted by direct comparison method against Pressure Measuring Instruments Standard according to calibration procedure CP-P04, using " DKD-R 6-1 ; Calibration of Pressure Gauges " as a guidelines.

Condition of this result of calibration

1.Reference standards instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Certificate No.</u>	<u>Due Date</u>
1) Pressure Calibrator	PC106P	1189	MP-0176-23	12 Sep 2024

2.This instrument was installed in vertical orientation and lower groove of pressure sensor was used as the reference level.

3.This result of calibration was made on requested at the point specified by customer.

4.Scale and conversion factor is 1 kPa = 7.50062 mmHg


5.This instrument was used clean air as pressure media.


6.This instrument was calibrated by applied pressure to high-port (+) side and low-port (-) side open to atmospheric pressure.

7.The certificate is valid only to the item calibrated on date and place of calibration.

8.This Certification is traceable to the International System of Unit maintained through:-

-National Institute of Metrology (Thailand), NSC-ONSC Accredited No. Calibration 0144

Calibrated by : 
Issue Date : 19 January 2024

Approved Signatory : 
☐ Phalinee Prabpaipal
☐ Sura Suwannasri
☒ Attapol Panurach



Cert.No.: 24P202

Page: 2 of 2

Result of calibration:- Without adjustment

Range : 0 mmHg to 1034 mmHg

Function:- Pressure Measurement

Resolution : 1 mmHg

Increasing Pressure

Applied Pressure (mmHg)	0.0	99.8	199.8	299.7	399.7	499.7	599.7	699.6	799.6	899.5	1033.4
UUC* Indication (mmHg)	0	99	198	298	398	497	597	697	797	897	1030
Error (mmHg)	0.0	-0.8	-1.8	-1.7	-1.7	-2.7	-2.7	-2.6	-2.6	-2.5	-3.4

Decreasing Pressure

Applied Pressure (mmHg)	1033.4	899.5	799.6	699.6	599.7	499.7	399.7	299.7	199.8	99.8	0.0
UUC* Indication (mmHg)	1030	897	797	697	597	497	398	298	198	99	0
Error (mmHg)	-3.4	-2.5	-2.6	-2.6	-2.7	-2.7	-1.7	-1.7	-1.8	-0.8	0.0

The uncertainty of measurement was ± 1.0 mmHg

* UUC = Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95 %.

-o0o-



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG, BANGKOK 10250
TEL. 0-2717-3000-24 FAX. 0-2719-9484



Certificate of Calibration

Certificate No. : 24P205

Page : 1 of 2

Equipment : Barometer

Manufacturer: Barigo

Model : -

Serial No.: -

ID No.: BM-06

Condition As-Received: Used Item

Received Date: 12 January 2024

Calibration Date: 17 January 2024

Reference: 2401-0387WN

Submitted by: LIFE & ENVIRONMENT CO., LTD.

Ambient Temperature: (23 ± 2) °C

Relative Humidity: (50 ± 15) %

Atmospheric Pressure: 1013 mbar

This certificate may not be reproduced other than in full,
except with the prior written approval of the head of
Corporate Services 3: Equipment Calibration and Testing Services.

90, 92, 94 Soi On-Nuch 64, Srinakarin Road,
On-Nuch, Suanluang, Bangkok 10250

Procedure used: The calibration was conducted by direct comparison method against Pressure Measuring Instruments Standard according to calibration procedure CP-P10, using " DKD-R 6-1 ; Calibration of Pressure Gauges " as a guidelines.

Condition of this result of calibration

1.Reference standards instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Certificate No.</u>	<u>Due Date</u>
1) Standard Barometer	DPI142	1422505046	MP-0094-23	03 May 2024

2.This instrument was installed in vertical orientation and center of the dial was used as the reference level.

3.This result of calibration was made on requested at the point specified by customer.

4.Scale and conversion factor is 1 kPa = 7.50062 mmHg

5.This result of calibration instrument was in absolute pressure.

6.This instrument was used clean air as pressure media.

7.The certificate is valid only to the item calibrated on date and place of calibration.

8.This Certification is traceable to the International System of Unit maintained through:-

-National Institute of Metrology Thailand (NIMT)

Calibrated by :

Issue Date : 18 January 2024

Approved Signatory :

[] Phalinee Prabpaipal

[] Sura Suwannasri

☒ Attapoi Panurach



Cert.No.: 24P205

Page: 2 of 2

Result of calibration:- Without adjustment

Range : 730 mmHg to 770 mmHg

Function:- Absolute Pressure Measurement

Scale Interval : 1 mmHg (The Fifth Estimate)

Increasing Pressure

Applied Pressure (mmHg)	735.17	744.69	753.26	761.80	770.67
UUC* Indication (mmHg)	730.0	740.0	750.0	760.0	770.0
Error (mmHg)	-5.17	-4.69	-3.26	-1.80	-0.67

Decreasing Pressure

Applied Pressure (mmHg)	770.67	760.89	751.95	743.88	735.28
UUC* Indication (mmHg)	770.0	760.0	750.0	740.0	730.0
Error (mmHg)	-0.67	-0.89	-1.95	-3.88	-5.28

The uncertainty of measurement was ± 0.24 mmHg

* UUC = Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95 %.

-o0o-

Certificate No: G 670046

Date of issue : 23-Jan-24

Instrument description : Gas Analyzer
Instrument model : EC 9832 Series CO
Control unit serial no. : -
Instrument serial no. : 13-1210
ID no. or control no. : -
Manufacturer : Ecotech
Probe description : -
Probe model : -
Probe serial no. : -
Customer name : Life & Environment Co., Ltd. (Head Office)
Customer address : 90,92,94 Soi On-Nuch 64, Srinakarin Road, Suanluang, Bangkok 10250

Total pages of certificate : 2 Pages
Receiving no. : L-240219
Receiving date. : 22-Jan-24
Parameter of calibration : Gas Calibration(Carbon Monoxide 1003 ppm)
Condition of UUC. : Used
Ambient condition : All of the Measurment ware caried out the stabilized labotary

Temperature : 23 ±5 °C

Humidity : 55 ± 15 %RH

Calibration place : 17/121 Soi Ngamwongwan 47 Yaek 48, Toongsonghong, Laksi, Bangkok 10210

Calibration procedure no. : This instrument was calibrated by comparison with Standard gas mixture according to calibration Work Instruction no. WI-CL-19-C

The calibration certificate expanded uncertainty of measurement is stated as the standard uncertainty of measurent Multiplied by coverage factor $k=2$, which for a normal distribution corresponds to a coverage probability of approximately 95%.

This certificate is applied only to item under test Environmental condition.


This Calibration Certificate may not be reporduced other than in full except with the permission of the issuing laboratory. Calibration certificates without signature and seal not valid and The results relate only to the items tested/calibrated.

This calibration certificate documents are tracebility to national standards, which realize measurement according to the International System of Units (SI).

Date of calibration : 23-Jan-24



Calibration Technician

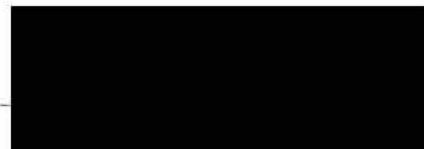

Technical Manager

Certificate No.: G 670046

Standard References (Table 1)

Standard	Certificate No.	Vendor	Due date
Carbon monoxide (CO) 1003 ppm	2584/23	Linde	10-Sep-25

Measured room conditions

Temperature : 22.9 °C Humidity : 60.3 %RH Pressure : 1012.8 mbar

Calibration conditions

Gas Temperature : 23 °C Flow rate : 1,500 ml/min Gas pressure : 1018.4 mbar

Calibration Results (Without adjustment) (Table 2)

Parameter of Standard	Standard Values	Mean of UUC	Error	Uncertainty (±)
CO (ppm)	1003	1219.99	216.99	12

Remark : 1 µmol/mol = 1 ppm.

End of Report

Testing Report

General Information

Measuring Site : Entech Industrial Solution Co.,Ltd. Report No. : R 670002
Address : 17/121 Soi Ngamwongwan 47 Yaek 48 , Toongsonghong, Laksi, Bangkok 10210 THAILAND Date of Issue : 20-Feb-24
Parameter : Gas Date of testing : 20-Feb-24

Customer Devices Information

Instrument Description : Flue Gas Analyzer
Instrument Model : Testo 330-1LL
Instrument S/N : 01688735
ID no. Or Control no. : -
Manufacturer : Testo SE & Co. KGaA
Receiving no : L-240646

Standard Reference

Standard	Reference No.	Traceability	Due Date
Oxygen (O ₂) 2.50 % Vol	2412/23	Linde	27-Aug-27
Oxygen (O ₂) 10.04 % Vol	CG-0153-21	Nimt	18-Nov-26
Oxygen (O ₂) 21.02 % Vol	CG-0041-22	Nimt	10-Feb-27
Carbon Monoxide (CO) 80.14 ppm	CG-0040-22	Nimt	14-Feb-27
Carbon Monoxide (CO) 302 ppm	1915/23	Linde	16-Jun-25
Carbon Monoxide (CO) 1003 ppm	2584/23	Linde	10-Sep-25

Results : The testing results were reported in the table below

No.	Gas	Standard Gas	UUT Mean	Error
1	O ₂	2.50	2.6	0.10
2	O ₂	10.04	10.2	0.16
3	O ₂	21.02	21.2	0.18
4	CO	80.14	79	-1.14
5	CO	302	302	0
6	CO	1003	1001	-2

Tested by

Approved by





TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3 : EQUIPMENT CALIBRATION AND TESTING SERVICES

534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250

TEL. 0-2717-3000-29 FAX. 0-2719-9484

Cert.No.: 24CH37

Page.: 1 of 2

Certificate of Calibration

Equipment :	pH Meter
Manufacturer :	Hanna
Model :	HI 3222
Serial No. :	08645111
ID No. :	-
Condition As-Received:	Used Item
Received Date :	09 January 2024
Calibration Date :	10 January 2024
Reference :	2401-0234WN-1
Submitted by :	LIFE & ENVIRONMENT CO., LTD. 90, 92, 94 Soi On-Nuch 64, Srinakarin Road, On-Nuch, Suanluang, Bangkok 10250
Ambient Temperature :	(25 ± 2.5) °C
Relative Humidity :	(50 ± 15) %
Calibration Procedure :	In - house method : - CP-CH5 by direct measurement with standard voltage calibrator and direct measurement with certified reference material (CRM)

Calibrated by :

Approved by :

(✓)
()
()



Issue Date :

12 January 2024

Approved Signatory

The Uncertainties are for a confidence probability of approximately 95%.

This certificate may not be reproduced other than in full, except with the prior written approval of the head of Calibration and Testing Equipment Services.

A 0012728



Cert. No.: 24CH37

Page.: 2 of 2

Condition of this calibration result

1. Reference Standard Instrument : -

<u>Instrument</u>	<u>Serial No.</u>	<u>ID No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
1) Document Process Calibrator	54030049	130RC116	23E2802	27 Aug 2024

This certification is traceable to the International System of Unit maintained through:-

- Technology Promotion Association (Thailand-Japan)

2. Certified Reference Materials : The measurement results are traceable to SI through CPA chem Ltd.,
ANSI-ASQ National Accreditation Board, Accredited No. AR-1835

<u>Buffer Solution</u>	<u>Manufacturer</u>	<u>Lot No.</u>	<u>Exp. date</u>
pH 4.008	CPA chem	940102	27 Nov 2025
pH 6.986	CPA chem	931959	01 Oct 2024
pH 9.997	CPA chem	940106	02 Nov 2024

3. This certificate is valid only to the item calibrated on date and place of calibration.

Calibration Results

Function : mV Measurement

Performing standard curve by Fluke at pH (4,7,10)

Unit Under Calibration	Nominal Value	Standard Voltage Input	Actual Reading		Uncertainty of Measurement (±mV)	Coverage factor k
	pH	mV	mV	pH		
pH Meter S/N.: 08645111	4.000	177.48	177.3	4.000	0.058	2.00
	7.000	0.00	-0.1	7.000	0.058	2.00
	10.000	-177.48	-177.5	10.000	0.058	2.00

Function : pH Measurement

Performing three buffers standard curve by using buffer nominal pH (4,7,10)

Unit Under Calibration	Standard pH Buffer Solution	Actual pH Reading	Actual mV Reading (mV)	Uncertainty of pH measurement (±)	Coverage factor k
pH Electrode S/N.: 092818FN	4.008	4.011	167.5	0.0045	2.00
	6.986	7.006	-7.6	0.0084	2.00
	9.997	9.997	-181.7	0.0065	2.00

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k , providing a level of confidence of approximately 95 %.

-o0o-



Certificate of Calibration

Equipment:	Cooled Incubator	Certificate No.:	C31232288
Model:	i250	Issued Date:	14 November 2023
Serial No.(or ID):	0812-0416 (W-BOD-01/55)	Job No.:	WO-00008954
Manufacturer:	Accuplus	Page:	1 of 3
Condition:	In Condition	Ventilation Valve:	None
Shelves(pc.):	2		

Customer: LIFE & ENVIRONMENT CO., LTD.
90, 92, 94 Soi On-nuch 64, Srinakarin Road, On-nuch,
Suanluang, Bangkok 10250 Thailand

Environment Condition:

Temperature:	21 °C	±	1.4 °C
Humidity:	61 %RH	±	5.2 %RH
Voltage:	229 VAC	±	2.9 VAC


Calibration Place: LIFE & ENVIRONMENT CO., LTD. (Water & Soil Testing Laboratory)
90, 92, 94 Soi On-nuch 64, Srinakarin Road, On-nuch,
Suanluang, Bangkok 10250 Thailand

Calibration By: Mr. Suphanimit Khamnonphoem
Calibration Date: 06 November 2023
The Method used: In house method, CAL-WI-16, base on TLAS-G20

Traceability: This certificate is traceable to the SI Units maintained by National Institute of Metrology (NIMT), Thailand through DKSH Technology Limited.
Certificate No. C10230012



Person in charge

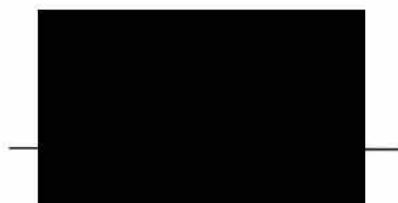


Authorized signatory

This certificate is issued the units of measurement according to the International System of Units (SI). It provides traceability of measurement to international or national standard or other recognized national standard laboratories.

The measurement uncertainty stated is the expanded uncertainty which is obtained from the standard uncertainty multiplied by the coverage factor (k=2) to provide a level of confidence of approximately 95%. It is determined in accordance with the Guide to Expression of Uncertainty in Measurement (GUM).

These results may be affected by deviations from specified conditions. The results relate only to the items tested, calibrated or sampled. The report shall not be reproduced except in full without approval of DKSH Technology Limited.

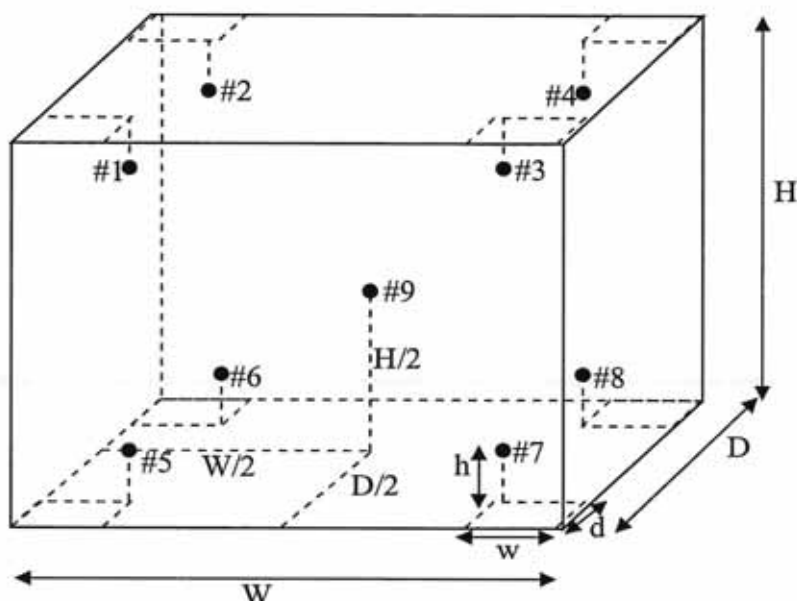

Standard Installation Locations

Volume (Calibration Zone)= 102 (Liters)

Inside chamber: $W = 50$ (cm) $D = 50$ (cm) $H = 104$ (cm)

Standard Locations (#1, #2, #3, #4): $w = 5$ (cm) $d = 5$ (cm) $h = 30$ (cm)

Standard Locations (#5, #6, #7, #8): $w = 5$ (cm) $d = 5$ (cm) $h = 10$ (cm)

#9: Geometric center of the chamber

Position of Std	#1	#2	#3	#4	#5	#6	#7	#8	#9
Channel of Logger	101	102	103	104	105	106	107	108	109

Definitions

Indicating Temperature: The average reading of indicating device which forms the integral part of the enclosure.

Measured Temperature: The average reading of standards at any positions or location.

Measured Uniformity: The maximum difference of measured temperatures between of any probes and the measured temperature at the reference location which are observed at same time or at close observation time as possible to determine the temperature pattern or homogeneity with the chamber at steady-state. The reference probe is preferably located in the geometric center of the chamber.

Measured Stability: The one-half of greatest maximum difference of measured temperatures at any one probe.

Overall Variation: The difference of maximum and minimum measured temperatures throughout observation time.

Calibration Results:

Without adjustment

Measurement Temperature at Spread Locations, Indicating of Unit Under Calibration: 20.0 °C

Locations	Measured Temperature (°C)	Correction of UUC. (°C)	Uncertainty (± °C)
#1	20.20	0.20	0.23
#2	20.38	0.38	0.24
#3	20.01	0.01	0.23
#4	20.26	0.26	0.23
#5	19.98	-0.02	0.26
#6	20.15	0.15	0.23
#7	20.02	0.02	0.26
#8	19.84	-0.16	0.23
#9	20.26	0.26	0.23

Temperature Distribution

Desired (°C)	Setting (°C)	Indicating (°C)	Measured Temperature at Spread Locations (°C)									Uncertainty (± °C)*
			#1	#2	#3	#4	#5	#6	#7	#8	#9	
20.0	20.0	20.0	20.20	20.38	20.01	20.26	19.98	20.15	20.02	19.84	20.26	0.26

Chamber Characterization

Indicating (°C)	Measured Uniformity (°C)	Measured Stability (± °C)	Overall Variation (°C)
20.0	0.45	0.13	0.71

Note: * Maximum uncertainty of the each position

The End of Certificate

Certificate of Calibration

Equipment:	COD Reactor	Certificate No.:	C17240092
Model:	HI 839150-02	Issued Date:	13 June 2024
Serial No. (or ID.):	101380040111	Job No.:	WO-00030976
Manufacturer:	HANNA	Page:	1 of 4
Condition:	In Condition		
Covers: Open (Max)	Locations heating Block: Single		

Customer: LIFE & ENVIRONMENT CO., LTD.
90, 92, 94 Soi On-nuch 64, Srinakarin Road,
On-nuch, Suanluang, Bangkok 10250 Thailand

Environment Condition: Temperature: 23 °C ± 5.0 °C
Humidity: 50 %RH ± 15.0 %RH
Voltage: 230 VAC ± 11.0 VAC

Calibration Place: Temperature Laboratory, DKSH Technology Limited.
2533 Sukhumvit Road, Bangchak,
Phrakhanong, Bangkok 10260 Thailand

Calibration By: Mr. Vanasapol Lerksanthia


Calibration Date: 13 June 2024

The Method used: In house method, CAL-WI-59, base on Direct Measurement with Standard Thermometer

Traceability: This certificate is traceable to the SI Units maintained by National Institute of Metrology (NIMT), Thailand through DKSH Technology Limited.
Certificate No. C10240011



Person in charge

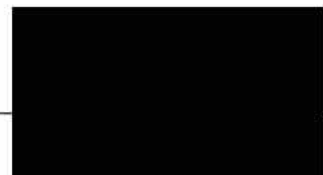


Authorized signatory


This certificate is issued the units of measurement according to the International System of Units (SI). It provides traceability of measurement to international or national standard or other recognized national standard laboratories.

The measurement uncertainty stated is the expanded uncertainty which is obtained from the standard uncertainty multiplied by the coverage factor ($k=2$) to provide a level of confidence of approximately 95%. It is determined in accordance with the Guide to Expression of Uncertainty in Measurement (GUM).

These results may be affected by deviations from specified conditions. The results relate only to the items tested, calibrated or sampled. The report shall not be reproduced except in full without approval of DKSH Technology Limited.

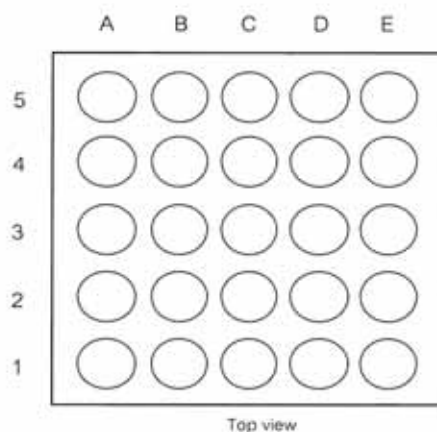

Location of standard

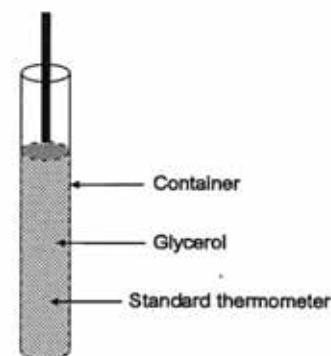

Sample test

Standard Installation Locations

The standard thermometer touches the lower end of the boring

Definitions

- Indicating Temperature:** The average reading of indicating device which forms the integral part of the unit under calibration.
- Measured Temperature:** The average reading of standards at any positions or location.
- Measured Stability:** The one-half of greatest maximum difference of measured temperatures at any one probe.

Calibration Results:

Without Adjustment

Measured temperature at the spread locations:

Locations heating Block:	Setting (°C)	Unit Under Calibration (°C)
Single	150.0	150.0

Location heating Block:	Measured Temperature (°C)	Correction of UUC (°C)	Uncertainty (± °C)
A1	149.14	-0.86	0.33
A2	150.86	0.86	0.34
A3	149.81	-0.19	0.37
A4	148.95	-1.05	0.42
A5	149.83	-0.17	0.38
B1	149.16	-0.84	0.37
B2	150.42	0.42	0.50
B3	151.11	1.11	0.48
B4	150.07	0.07	0.57
B5	149.25	-0.75	0.52
C1	149.51	-0.49	0.45
C2	151.09	1.09	0.55
C3	151.12	1.12	0.43
C4	149.70	-0.30	0.41
C5	149.53	-0.47	0.51
D1	149.29	-0.71	0.45
D2	150.91	0.91	0.55
D3	151.07	1.07	0.43
D4	149.88	-0.12	0.41
D5	149.47	-0.53	0.51
E1	149.38	-0.62	0.45
E2	150.96	0.96	0.55
E3	150.75	0.75	0.43
E4	149.82	-0.18	0.42
E5	149.63	-0.37	0.51

Characterization of the unit under calibration:

Locations heating Block	Desired	Unit Under Calibration (°C)		Measured Temperature (°C)
	(°C)	Setting	Reading	Stability (±°C)
Single	150.0	150.0	150.0	0.43

The End of Certificate



Certificate of Calibration

Equipment:	Cooled Incubator	Certificate No.:	C31232287
Model:	i250	Issued Date:	14 November 2023
Serial No.(or ID):	0812-0414 (W-RE-01/55)	Job No.:	WO-00008954
Manufacturer:	Accuplus	Page:	1 of 3
Condition:	In Condition	Ventilation Valve:	None
Shelves(pc.):	2		

Customer: LIFE & ENVIRONMENT CO., LTD.
90, 92, 94 Soi On-nuch 64, Srinakarin Road, On-nuch,
Suanluang, Bangkok 10250 Thailand

Environment Condition:

Temperature:	21 °C	±	1.4 °C
Humidity:	61 %RH	±	5.2 %RH
Voltage:	229 VAC	±	2.9 VAC

Calibration Place: LIFE & ENVIRONMENT CO., LTD. (Water & Soil Testing Laboratory)
90, 92, 94 Soi On-nuch 64, Srinakarin Road, On-nuch,
Suanluang, Bangkok 10250 Thailand

Calibration By: Mr. Suphanimit Khamnonphoem


Calibration Date: 06 November 2023

The Method used: In house method, CAL-WI-16, base on TLAS-G20

Traceability: This certificate is traceable to the SI Units maintained by National Institute of Metrology (NIMT), Thailand through DKSH Technology Limited.
Certificate No. C10230012



Person in charge

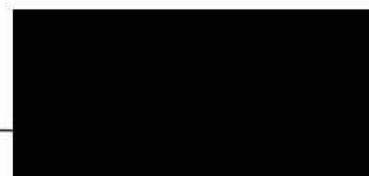


Authorized signatory

This certificate is issued the units of measurement according to the International System of Units (SI). It provides traceability of measurement to international or national standard or other recognized national standard laboratories.

The measurement uncertainty stated is the expanded uncertainty which is obtained from the standard uncertainty multiplied by the coverage factor ($k=2$) to provide a level of confidence of approximately 95%. It is determined in accordance with the Guide to Expression of Uncertainty in Measurement (GUM).

These results may be affected by deviations from specified conditions. The results relate only to the items tested, calibrated or sampled. The report shall not be reproduced except in full without approval of DKSH Technology Limited.

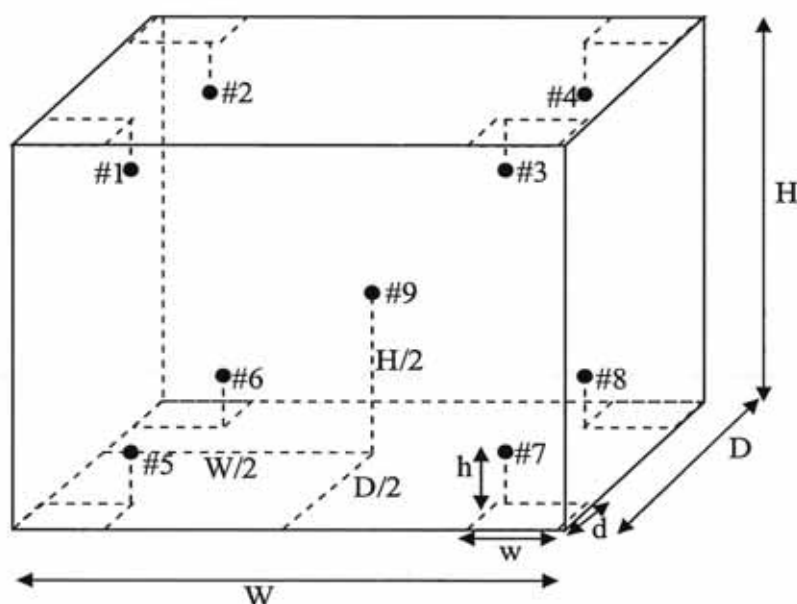

Standard Installation Locations

Volume (Calibration Zone)= 102 (Liters)

Inside chamber:	W = 50 (cm)	D = 50 (cm)	H = 104 (cm)
Standard Locations (#1, #2, #3, #4):	w = 5 (cm)	d = 5 (cm)	h = 30 (cm)
Standard Locations (#5, #6, #7, #8):	w = 5 (cm)	d = 5 (cm)	h = 10 (cm)

#9: Geometric center of the chamber

Position of Std	#1	#2	#3	#4	#5	#6	#7	#8	#9
Channel of Logger	201	202	203	204	205	206	207	208	209

Definitions

Indicating Temperature: The average reading of indicating device which forms the integral part of the enclosure.

Measured Temperature: The average reading of standards at any positions or location.

Measured Uniformity: The maximum difference of measured temperatures between of any probes and the measured temperature at the reference location which are observed at same time or at close observation time as possible to determine the temperature pattern or homogeneity with the chamber at steady-state. The reference probe is preferably located in the geometric center of the chamber.

Measured Stability: The one-half of greatest maximum difference of measured temperatures at any one probe.

Overall Variation: The difference of maximum and minimum measured temperatures throughout observation time.

Calibration Results:

Without adjustment

Measurement Temperature at Spread Locations, Indicating of Unit Under Calibration: 4.0 °C

Locations	Measured Temperature (°C)	Correction of UUC. (°C)	Uncertainty (± °C)
#1	3.79	-0.21	0.79
#2	3.56	-0.44	0.92
#3	4.05	0.05	0.67
#4	3.84	-0.16	0.84
#5	4.12	0.12	0.45
#6	3.80	-0.20	0.74
#7	3.99	-0.01	0.52
#8	4.09	0.09	0.51
#9	3.69	-0.31	0.75

Temperature Distribution


Desired (°C)	Setting (°C)	Indicating (°C)	Measured Temperature at Spread Locations (°C)									Uncertainty (± °C)*
			#1	#2	#3	#4	#5	#6	#7	#8	#9	
4.0	4.0	4.0	3.79	3.56	4.05	3.84	4.12	3.80	3.99	4.09	3.69	0.92

Chamber Characterization

Indicating (°C)	Measured Uniformity (°C)	Measured Stability (± °C)	Overall Variation (°C)
4.0	0.75	0.75	1.72

Note: * Maximum uncertainty of the each position

The End of Certificate

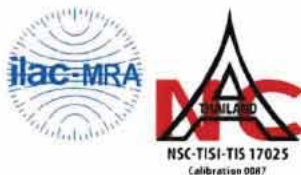

Certificate of Calibration

Equipment:	Cooled Incubator	Certificate No.:	C31242227
Model:	i250	Issued Date:	08 November 2024
Serial No.(or ID):	0812-0414 (W-RE-01/55)	Job No.:	WO-00047861
Manufacturer:	Accuplus	Page:	1 of 3
Condition:	In Condition	Ventilation Valve:	None
Shelves(pc.):	2		

Customer: LIFE & ENVIRONMENT CO., LTD.
90, 92, 94 Soi On-nuch 64, Srinakarin Road, On-nuch,
Suanluang, Bangkok 10250 Thailand


Environment Condition:

Temperature:	26 °C	±	0.5 °C
Humidity:	51 %RH	±	5.2 %RH
Voltage:	229 VAC	±	2.0 VAC


Calibration Place: LIFE & ENVIRONMENT CO., LTD. (Water & Soil Testing Laboratory)
90, 92, 94 Soi On-nuch 64, Srinakarin Road, On-nuch,
Suanluang, Bangkok 10250 Thailand

Calibration By: Mr. Suphanimit Khamnonphoem
Calibration Date: 05 November 2024
The Method used: In house method, CAL-WI-16, base on TLAS-G20

Traceability: This certificate is traceable to the SI Units maintained by National Institute of Metrology (NIMT), Thailand through DKSH Technology Limited.
Certificate No. C10240015



Person in charge

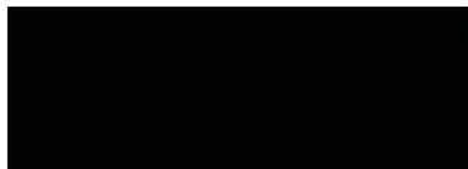


Authorized signatory

This certificate is issued the units of measurement according to the International System of Units (SI). It provides traceability of measurement to international or national standard or other recognized national standard laboratories.

The measurement uncertainty stated is the expanded uncertainty which is obtained from the standard uncertainty multiplied by the coverage factor (k=2) to provide a level of confidence of approximately 95%. It is determined in accordance with the Guide to Expression of Uncertainty in Measurement (GUM).

These results may be affected by deviations from specified conditions. The results relate only to the items tested, calibrated or sampled. The report shall not be reproduced except in full without approval of DKSH Technology Limited.

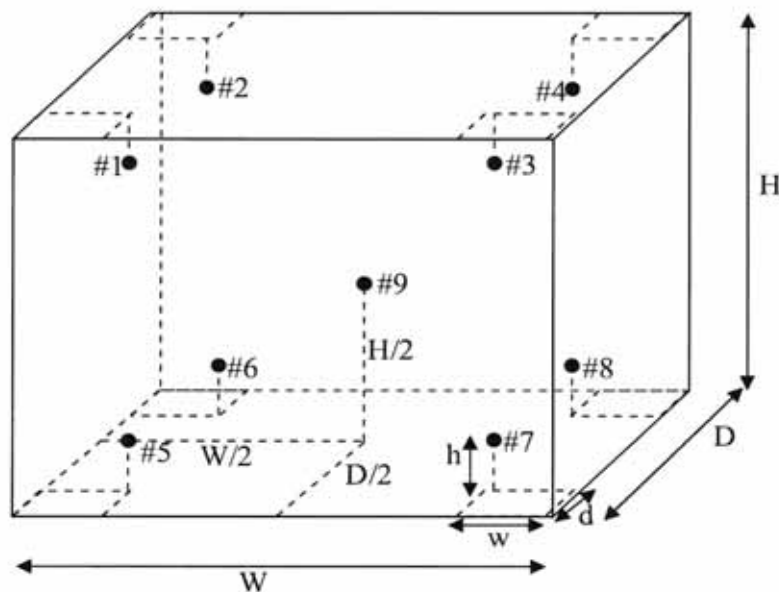

Standard Installation Locations

Volume (Calibration Zone)= 102 (Liters)

Inside chamber: $W = 50$ (cm) $D = 50$ (cm) $H = 104$ (cm)

Standard Locations (#1, #2, #3, #4): $w = 5$ (cm) $d = 5$ (cm) $h = 30$ (cm)

Standard Locations (#5, #6, #7, #8): $w = 5$ (cm) $d = 5$ (cm) $h = 10$ (cm)

#9: Geometric center of the chamber

Position of Std	#1	#2	#3	#4	#5	#6	#7	#8	#9
Channel of Logger	201	202	203	204	205	206	207	208	209

Definitions

Indicating Temperature: The average reading of indicating device which forms the integral part of the enclosure.

Measured Temperature: The average reading of standards at any positions or location.

Measured Uniformity: The maximum difference of measured temperatures between of any probes and the measured temperature at the reference location which are observed at same time or at close observation time as possible to determine the temperature pattern or homogeneity with the chamber at steady-state. The reference probe is preferably located in the geometric center of the chamber.

Measured Stability: The one-half of greatest maximum difference of measured temperatures at any one probe.

Overall Variation: The difference of maximum and minimum measured temperatures throughout observation time.

Calibration Results:
Without adjustment

Measurement Temperature at Spread Locations, Indicating of Unit Under Calibration: 4.0 °C

Locations	Measured Temperature (°C)	Correction of UUC. (°C)	Uncertainty (± °C)
#1	3.67	-0.33	0.81
#2	3.47	-0.53	0.89
#3	4.18	0.18	0.67
#4	3.80	-0.20	0.96
#5	4.23	0.23	0.51
#6	3.92	-0.08	0.68
#7	3.85	-0.15	0.66
#8	4.08	0.08	0.59
#9	3.85	-0.15	0.60

Temperature Distribution

Desired (°C)	Setting (°C)	Indicating (°C)	Measured Temperature at Spread Locations (°C)									Uncertainty (± °C)*
			#1	#2	#3	#4	#5	#6	#7	#8	#9	
4.0	4.0	4.0	3.67	3.47	4.18	3.80	4.23	3.92	3.85	4.08	3.85	0.96

Chamber Characterization

Indicating (°C)	Measured Uniformity (°C)	Measured Stability (± °C)	Overall Variation (°C)
4.0	0.69	0.80	1.89

Note: * Maximum uncertainty of the each position

The End of Certificate



Certificate of Calibration

Equipment:	Incubator	Certificate No.:	C31232289
Model:	INE 400	Issued Date:	14 November 2023
Serial No.(or ID):	E407.1277 (WM-IB-02/51)	Job No.:	WO-00008954
Manufacturer:	Memmert	Page:	1 of 3
Condition:	In Condition	Ventilation Valve:	Closed
Shelves(pc.):	1		

Customer: LIFE & ENVIRONMENT CO., LTD.
90, 92, 94 Soi On-nuch 64, Srinakarin Road,
Suanluang, Bangkok 10250 Thailand

Environment Condition:

Temperature:	24 °C	±	0.6 °C
Humidity:	50 %RH	±	4.4 %RH
Voltage:	224 VAC	±	2.5 VAC

Calibration Place: LIFE & ENVIRONMENT CO., LTD. (Microbiological Laboratory)
90, 92, 94 Soi On-nuch 64, Srinakarin Road,
Suanluang, Bangkok 10250 Thailand

Calibration By: Mr. Suphakorn Sookmee


Calibration Date: 06 November 2023

The Method used: In house method, CAL-WI-16, base on TLAS-G20

Traceability: This certificate is traceable to the SI Units maintained by National Institute of Metrology (NIMT), Thailand through DKSH Technology Limited.
Certificate No. C10230019



Person in charge

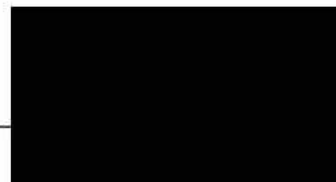


Authorized signatory

This certificate is issued the units of measurement according to the International System of Units (SI). It provides traceability of measurement to international or national standard or other recognized national standard laboratories.

The measurement uncertainty stated is the expanded uncertainty which is obtained from the standard uncertainty multiplied by the coverage factor ($k=2$) to provide a level of confidence of approximately 95%. It is determined in accordance with the Guide to Expression of Uncertainty in Measurement (GUM).

These results may be affected by deviations from specified conditions. The results relate only to the items tested, calibrated or sampled. The report shall not be reproduced except in full without approval of DKSH Technology Limited.

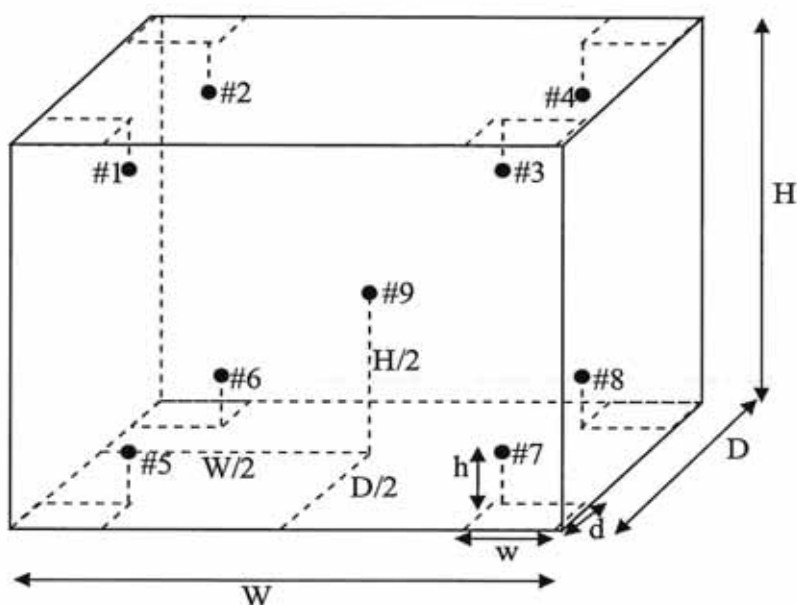

Standard Installation Locations

Volume (Calibration Zone)= 21 (Liters)

Inside chamber: $W = 40$ (cm) $D = 33$ (cm) $H = 40$ (cm)

Standard Locations (#1, #2, #3, #4): $w = 5$ (cm) $d = 5$ (cm) $h = 5$ (cm)

Standard Locations (#5, #6, #7, #8): $w = 5$ (cm) $d = 5$ (cm) $h = 5$ (cm)

#9: Geometric center of the chamber

Position of Std	#1	#2	#3	#4	#5	#6	#7	#8	#9
Channel of Logger	101	102	103	104	105	106	107	108	109

Definitions

Indicating Temperature: The average reading of indicating device which forms the integral part of the enclosure.

Measured Temperature: The average reading of standards at any positions or location.

Measured Uniformity: The maximum difference of measured temperatures between of any probes and the measured temperature at the reference location which are observed at same time or at close observation time as possible to determine the temperature pattern or homogeneity with the chamber at steady-state. The reference probe is preferably located in the geometric center of the chamber.

Measured Stability: The one-half of greatest maximum difference of measured temperatures at any one probe.

Overall Variation: The difference of maximum and minimum measured temperatures throughout observation time.

Calibration Results:

Without adjustment

Measurement Temperature at Spread Locations, Indicating of Unit Under Calibration: 35.0 °C

Locations	Measured Temperature (°C)	Correction of UUC. (°C)	Uncertainty (± °C)
#1	35.16	0.16	0.27
#2	34.98	-0.02	0.29
#3	35.13	0.13	0.33
#4	34.98	-0.02	0.27
#5	35.51	0.51	0.33
#6	35.58	0.58	0.35
#7	35.63	0.63	0.30
#8	35.70	0.70	0.33
#9	35.00	0.00	0.28

Temperature Distribution


Desired (°C)	Setting (°C)	Indicating (°C)	Measured Temperature at Spread Locations (°C)									Uncertainty (± °C)*
			#1	#2	#3	#4	#5	#6	#7	#8	#9	
35.0	35.0	35.0	35.16	34.98	35.13	34.98	35.51	35.58	35.63	35.70	35.00	0.35

Chamber Characterization

Indicating (°C)	Measured Uniformity (°C)	Measured Stability (± °C)	Overall Variation (°C)
35.0	0.85	0.11	0.90

Note: * Maximum uncertainty of the each position

The End of Certificate

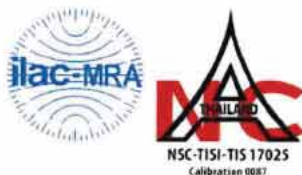

Certificate of Calibration

Equipment:	Incubator	Certificate No.:	C31242228
Model:	INE 400	Issued Date:	08 November 2024
Serial No.(or ID):	E407.1277 (WM-IB-02/51)	Job No.:	WO-00047861
Manufacturer:	Memmert	Page:	1 of 3
Condition:	In Condition	Ventilation Valve:	Closed
Shelves(pc.):	1		

Customer: LIFE & ENVIRONMENT CO., LTD.
90, 92, 94 Soi On-nuch 64, Srinakarin Road, On-nuch,
Suanluang, Bangkok 10250 Thailand

Environment Condition:

Temperature:	25 °C	±	1.3 °C
Humidity:	51 %RH	±	5.2 %RH
Voltage:	229 VAC	±	2.0 VAC


Calibration Place: LIFE & ENVIRONMENT CO., LTD. (Microbiological Laboratory)
90, 92, 94 Soi On-nuch 64, Srinakarin Road, On-nuch,
Suanluang, Bangkok 10250 Thailand

Calibration By: Mr. Suphanimit Khamnonphoem


Calibration Date: 05 November 2024

The Method used: In house method, CAL-WI-16, base on TLAS-G20

Traceability: This certificate is traceable to the SI Units maintained by National Institute of Metrology (NIMT), Thailand through DKSH Technology Limited.
Certificate No. C10240015



Person in charge

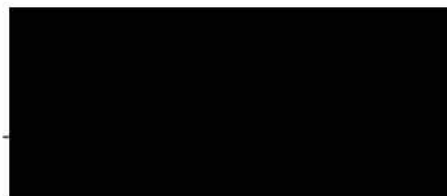


Authorized signatory

This certificate is issued the units of measurement according to the International System of Units (SI). It provides traceability of measurement to international or national standard or other recognized national standard laboratories.

The measurement uncertainty stated is the expanded uncertainty which is obtained from the standard uncertainty multiplied by the coverage factor (k=2) to provide a level of confidence of approximately 95%. It is determined in accordance with the Guide to Expression of Uncertainty in Measurement (GUM).

These results may be affected by deviations from specified conditions. The results relate only to the items tested, calibrated or sampled. The report shall not be reproduced except in full without approval of DKSH Technology Limited.

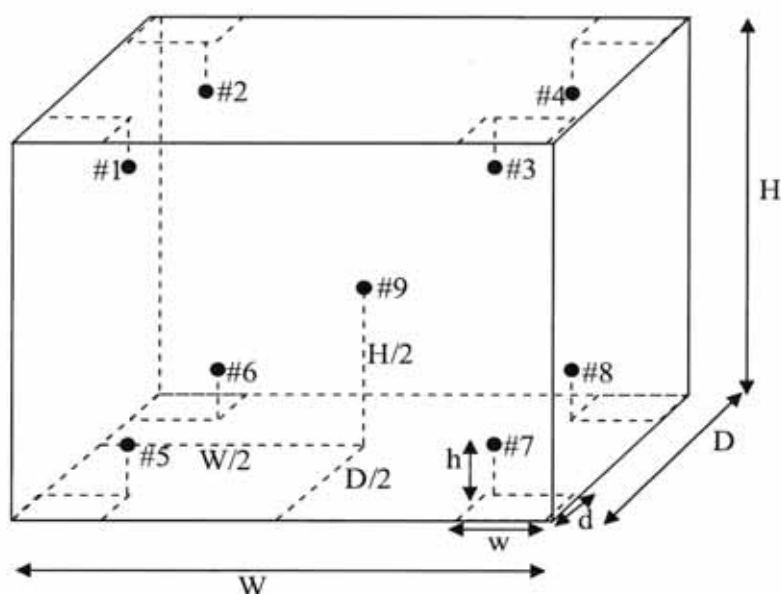

Standard Installation Locations

Volume (Calibration Zone)= 21 (Liters)

Inside chamber: $W = 40$ (cm) $D = 33$ (cm) $H = 40$ (cm)

Standard Locations (#1, #2, #3, #4): $w = 5$ (cm) $d = 5$ (cm) $h = 5$ (cm)

Standard Locations (#5, #6, #7, #8): $w = 5$ (cm) $d = 5$ (cm) $h = 5$ (cm)

#9: Geometric center of the chamber

Position of Std	#1	#2	#3	#4	#5	#6	#7	#8	#9
Channel of Logger	101	102	103	104	105	106	107	108	109

Definitions

Indicating Temperature: The average reading of indicating device which forms the integral part of the enclosure.

Measured Temperature: The average reading of standards at any positions or location.

Measured Uniformity: The maximum difference of measured temperatures between of any probes and the measured temperature at the reference location which are observed at same time or at close observation time as possible to determine the temperature pattern or homogeneity with the chamber at steady-state. The reference probe is preferably located in the geometric center of the chamber.

Measured Stability: The one-half of greatest maximum difference of measured temperatures at any one probe.

Overall Variation: The difference of maximum and minimum measured temperatures throughout observation time.

Calibration Results:
Without adjustment

Measurement Temperature at Spread Locations, Indicating of Unit Under Calibration: 35.0 °C

Locations	Measured Temperature (°C)	Correction of UUC. (°C)	Uncertainty (± °C)
#1	35.11	0.11	0.26
#2	34.95	-0.05	0.23
#3	35.02	0.02	0.24
#4	34.92	-0.08	0.23
#5	35.42	0.42	0.24
#6	35.29	0.29	0.25
#7	35.32	0.32	0.23
#8	35.38	0.38	0.25
#9	35.40	0.40	0.23

Temperature Distribution

Desired (°C)	Setting (°C)	Indicating (°C)	Measured Temperature at Spread Locations (°C)									Uncertainty (± °C)*
			#1	#2	#3	#4	#5	#6	#7	#8	#9	
35.0	35.0	35.0	35.11	34.95	35.02	34.92	35.42	35.29	35.32	35.38	35.40	0.26

Chamber Characterization

Indicating (°C)	Measured Uniformity (°C)	Measured Stability (± °C)	Overall Variation (°C)
35.0	0.55	0.07	0.56

Note: * Maximum uncertainty of the each position

The End of Certificate



Certificate of Calibration

Equipment:	Hot Air Oven	Certificate No.:	C31231015
Model:	UFE 400	Issued Date:	16 May 2023
Serial No.(or ID):	G412.0022	Job No.:	KSPR2307253
Manufacturer:	Memmert	Page:	1 of 5
Condition:	In Condition	Ventilation Valve:	Closed
Shelves(pc.):	1		

Customer: LIFE & ENVIRONMENT CO., LTD.
90, 92, 94 Soi On-nuch 64, Srinakarin Road,
On-nuch, Bangkok 10250 Thailand

Environment Condition:

Temperature:	27 °C	±	1.1 °C
Humidity:	58 %RH	±	5.2 %RH
Voltage:	224 VAC	±	1.4 VAC

Calibration Place: LIFE & ENVIRONMENT CO., LTD.(Water & Soil Testing Laboratory)
90, 92, 94 Soi On-nuch 64, Srinakarin Road,
On-nuch, Bangkok 10250 Thailand

Calibration By: Mr. Bovon Jannantha

Calibration Date: 16 May 2023

The Method used: In house method, CAL-WI-16, base on TLAS-G20

Traceability: This certificate is traceable to the SI Units maintained by National Institute of Metrology (NIMT), Thailand through DKSH Technology Limited.
Certificate No. C10230015



Person in charge




Authorized signatory

This certificate is issued the units of measurement according to the International System of Units (SI). It provides traceability of measurement to international or national standard or other recognized national standard laboratories.

The measurement uncertainty stated is the expanded uncertainty which is obtained from the standard uncertainty multiplied by the coverage factor ($k=2$) to provide a level of confidence of approximately 95%. It is determined in accordance with the Guide to Expression of Uncertainty in Measurement (GUM).

These results may be affected by deviations from specified conditions. The results relate only to the items tested, calibrated or sampled. The report shall not be reproduced except in full without approval of DKSH Technology Limited.

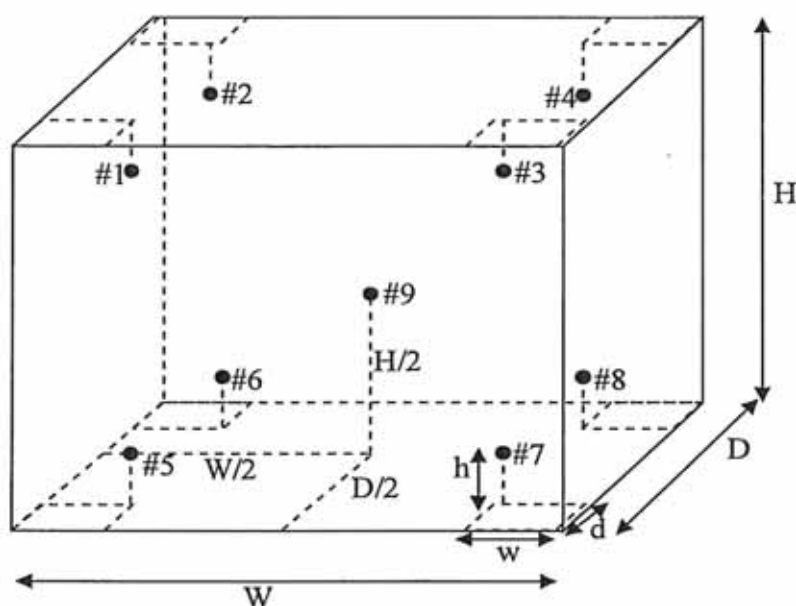

Standard Installation Locations

Volume (Calibration Zone)= 21 (Liters)

Inside chamber: $W = 40$ (cm) $D = 33$ (cm) $H = 40$ (cm)

Standard Locations (#1, #2, #3, #4): $w = 5$ (cm) $d = 5$ (cm) $h = 5$ (cm)

Standard Locations (#5, #6, #7, #8): $w = 5$ (cm) $d = 5$ (cm) $h = 5$ (cm)

#9: Geometric center of the chamber

Position of Std	#1	#2	#3	#4	#5	#6	#7	#8	#9
Channel of Logger	1	2	3	4	5	6	7	8	9

Definitions

Indicating Temperature: The average reading of indicating device which forms the integral part of the enclosure.

Measured Temperature: The average reading of standards at any positions or location.

Measured Uniformity: The maximum difference of measured temperatures between of any probes and the measured temperature at the reference location which are observed at same time or at close observation time as possible to determine the temperature pattern or homogeneity with the chamber at steady-state. The reference probe is preferably located in the geometric center of the chamber.

Measured Stability: The one-half of greatest maximum difference of measured temperatures at any one probe.

Overall Variation: The difference of maximum and minimum measured temperatures throughout observation time.

Calibration Results:

Without adjustment

Measurement Temperature at Spread Locations, Indicating of Unit Under Calibration: 104.0 °C

Locations	Measured Temperature (°C)	Correction of UUC. (°C)	Uncertainty (± °C)
#1	104.26	0.26	0.39
#2	104.22	0.22	0.39
#3	103.67	-0.33	0.39
#4	103.89	-0.11	0.39
#5	104.09	0.09	0.39
#6	103.69	-0.31	0.39
#7	103.98	-0.02	0.39
#8	104.11	0.11	0.39
#9	103.82	-0.18	0.39

Temperature Distribution

Desired (°C)	Setting (°C)	Indicating (°C)	Measured Temperature at Spread Locations (°C)									Uncertainty (± °C)*
			#1	#2	#3	#4	#5	#6	#7	#8	#9	
104.0	104.0	104.0	104.26	104.22	103.67	103.89	104.09	103.69	103.98	104.11	103.82	0.39

Chamber Characterization

Indicating (°C)	Measured Uniformity (°C)	Measured Stability (± °C)	Overall Variation (°C)
104.0	0.48	0.09	0.70

Note: * Maximum uncertainty of the each position

Without adjustment (Cont.)

Measurement Temperature at Spread Locations, Indicating of Unit Under Calibration: 150.0 °C

Locations	Measured Temperature (°C)	Correction of UUC. (°C)	Uncertainty (± °C)
#1	150.43	0.43	0.39
#2	150.43	0.43	0.39
#3	149.54	-0.46	0.39
#4	149.78	-0.22	0.39
#5	150.30	0.30	0.39
#6	149.56	-0.44	0.39
#7	149.86	-0.14	0.39
#8	150.05	0.05	0.39
#9	149.86	-0.14	0.39

Temperature Distribution

Desired (°C)	Setting (°C)	Indicating (°C)	Measured Temperature at Spread Locations (°C)									Uncertainty (± °C)*
			#1	#2	#3	#4	#5	#6	#7	#8	#9	
150.0	150.0	150.0	150.43	150.43	149.54	149.78	150.30	149.56	149.86	150.05	149.86	0.39

Chamber Characterization

Indicating (°C)	Measured Uniformity (°C)	Measured Stability (± °C)	Overall Variation (°C)
150.0	0.61	0.10	1.05

Note: * Maximum uncertainty of the each position

Without adjustment (Cont.)

Measurement Temperature at Spread Locations, Indicating of Unit Under Calibration: 180.0 °C

Locations	Measured Temperature (°C)	Correction of UUC. (°C)	Uncertainty (± °C)
#1	180.53	0.53	0.42
#2	180.59	0.59	0.42
#3	179.43	-0.57	0.42
#4	179.66	-0.34	0.42
#5	180.53	0.53	0.42
#6	179.48	-0.52	0.42
#7	179.93	-0.07	0.42
#8	180.10	0.10	0.42
#9	180.00	0.00	0.42

Temperature Distribution

Desired (°C)	Setting (°C)	Indicating (°C)	Measured Temperature at Spread Locations (°C)									Uncertainty (± °C)*
			#1	#2	#3	#4	#5	#6	#7	#8	#9	
180.0	180.0	180.0	180.53	180.59	179.43	179.66	180.53	179.48	179.93	180.10	180.00	0.42

Chamber Characterization

Indicating (°C)	Measured Uniformity (°C)	Measured Stability (± °C)	Overall Variation (°C)
180.0	0.67	0.08	1.30

Note: * Maximum uncertainty of the each position

The End of Certificate



Certificate of Calibration

Equipment:	Hot Air Oven	Certificate No.:	C31241025
Model:	UFE 400	Issued Date:	17 May 2024
Serial No.(or ID):	G412.0022	Job No.:	WO-00027714
Manufacturer:	Memmert	Page:	1 of 5
Condition:	In Condition	Ventilation Valve:	Closed
Shelves(pc.):	1		

Customer: LIFE & ENVIRONMENT CO., LTD.
90, 92, 94 Soi On-nuch 64, Srinakarin Road, On-nuch,
Suanluang, Bangkok 10250 Thailand

Environment Condition:

Temperature:	27 °C	±	1.0 °C
Humidity:	56 %RH	±	5.7 %RH
Voltage:	230 VAC	±	2.1 VAC

Calibration Place: LIFE & ENVIRONMENT CO., LTD. (Water & Soil Testing Laboratory)
90, 92, 94 Soi On-nuch 64, Srinakarin Road, On-nuch,
Suanluang, Bangkok 10250 Thailand

Calibration By: Mr. Nakarin Ruenros
Calibration Date: 16 May 2024
The Method used: In house method, CAL-WI-16, base on TLAS-G20

Traceability: This certificate is traceable to the SI Units maintained by National Institute of Metrology (NIMT), Thailand through DKSH Technology Limited.
Certificate No. C10230023



Person in charge




Authorized signatory

This certificate is issued the units of measurement according to the International System of Units (SI). It provides traceability of measurement to international or national standard or other recognized national standard laboratories.

The measurement uncertainty stated is the expanded uncertainty which is obtained from the standard uncertainty multiplied by the coverage factor (k=2) to provide a level of confidence of approximately 95%. It is determined in accordance with the Guide to Expression of Uncertainty in Measurement (GUM).

These results may be affected by deviations from specified conditions. The results relate only to the items tested, calibrated or sampled. The report shall not be reproduced except in full without approval of DKSH Technology Limited.

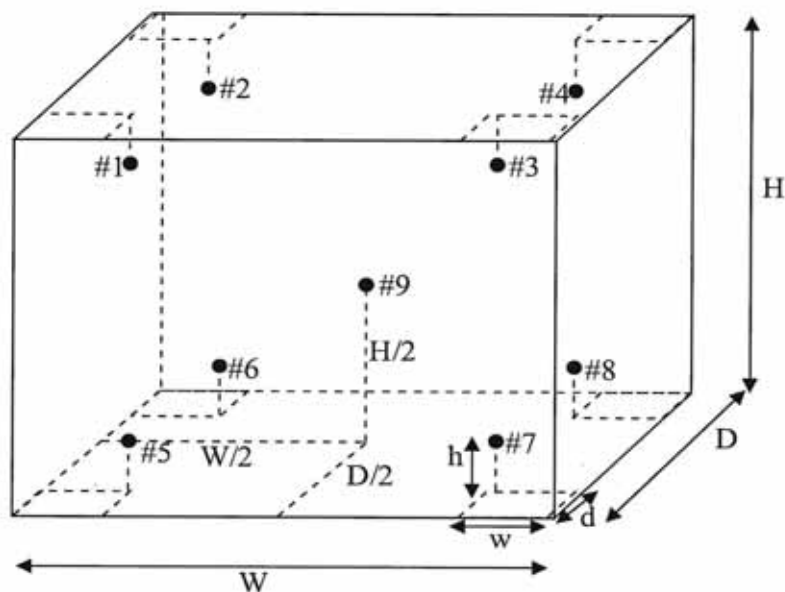

Standard Installation Locations

Volume (Calibration Zone)= 21 (Liters)

Inside chamber:	W = 40 (cm)	D = 33 (cm)	H = 40 (cm)
Standard Locations (#1, #2, #3, #4):	w = 5 (cm)	d = 5 (cm)	h = 5 (cm)
Standard Locations (#5, #6, #7, #8):	w = 5 (cm)	d = 5 (cm)	h = 5 (cm)

#9: Geometric center of the chamber

Position of Std	#1	#2	#3	#4	#5	#6	#7	#8	#9
Channel of Logger	101	102	103	104	105	106	107	108	109

Definitions

Indicating Temperature: The average reading of indicating device which forms the integral part of the enclosure.

Measured Temperature: The average reading of standards at any positions or location.

Measured Uniformity: The maximum difference of measured temperatures between of any probes and the measured temperature at the reference location which are observed at same time or at close observation time as possible to determine the temperature pattern or homogeneity with the chamber at steady-state. The reference probe is preferably located in the geometric center of the chamber.

Measured Stability: The one-half of greatest maximum difference of measured temperatures at any one probe.

Overall Variation: The difference of maximum and minimum measured temperatures throughout observation time.

Calibration Results:

Without adjustment

Measurement Temperature at Spread Locations, Indicating of Unit Under Calibration: 104.0 °C

Locations	Measured Temperature (°C)	Correction of UUC. (°C)	Uncertainty (± °C)
#1	104.27	0.27	0.39
#2	104.30	0.30	0.39
#3	103.80	-0.20	0.39
#4	104.15	0.15	0.39
#5	104.26	0.26	0.39
#6	104.15	0.15	0.39
#7	103.79	-0.21	0.39
#8	103.98	-0.02	0.39
#9	104.33	0.33	0.39

Temperature Distribution

Desired (°C)	Setting (°C)	Indicating (°C)	Measured Temperature at Spread Locations (°C)									Uncertainty (± °C)*
			#1	#2	#3	#4	#5	#6	#7	#8	#9	
104.0	104.0	104.0	104.27	104.30	103.80	104.15	104.26	104.15	103.79	103.98	104.33	0.39

Chamber Characterization

Indicating (°C)	Measured Uniformity (°C)	Measured Stability (± °C)	Overall Variation (°C)
104.0	0.65	0.10	0.72

Note: * Maximum uncertainty of the each position

Without adjustment (Cont.)

Measurement Temperature at Spread Locations, Indicating of Unit Under Calibration: 150.0 °C

Locations	Measured Temperature (°C)	Correction of UUC. (°C)	Uncertainty (± °C)
#1	150.35	0.35	0.39
#2	150.43	0.43	0.39
#3	149.42	-0.58	0.39
#4	150.13	0.13	0.39
#5	150.51	0.51	0.39
#6	150.30	0.30	0.39
#7	149.56	-0.44	0.40
#8	150.00	0.00	0.39
#9	150.33	0.33	0.39

Temperature Distribution

Desired (°C)	Setting (°C)	Indicating (°C)	Measured Temperature at Spread Locations (°C)									Uncertainty (± °C)*
			#1	#2	#3	#4	#5	#6	#7	#8	#9	
150.0	150.0	150.0	150.35	150.43	149.42	150.13	150.51	150.30	149.56	150.00	150.33	0.40

Chamber Characterization

Indicating (°C)	Measured Uniformity (°C)	Measured Stability (± °C)	Overall Variation (°C)
150.0	0.99	0.09	1.21

Note: * Maximum uncertainty of the each position

Without adjustment (Cont.)

Measurement Temperature at Spread Locations, Indicating of Unit Under Calibration: 180.0 °C

Locations	Measured Temperature (°C)	Correction of UUC. (°C)	Uncertainty (± °C)
#1	180.31	0.31	0.49
#2	180.46	0.46	0.49
#3	179.05	-0.95	0.50
#4	179.99	-0.01	0.49
#5	180.71	0.71	0.49
#6	180.36	0.36	0.50
#7	179.39	-0.61	0.50
#8	180.02	0.02	0.49
#9	180.51	0.51	0.50

Temperature Distribution

Desired (°C)	Setting (°C)	Indicating (°C)	Measured Temperature at Spread Locations (°C)									Uncertainty (± °C)*
			#1	#2	#3	#4	#5	#6	#7	#8	#9	
180.0	180.0	180.0	180.31	180.46	179.05	179.99	180.71	180.36	179.39	180.02	180.51	0.50

Chamber Characterization

Indicating (°C)	Measured Uniformity (°C)	Measured Stability (± °C)	Overall Variation (°C)
180.0	1.65	0.11	1.83

Note: * Maximum uncertainty of the each position

The End of Certificate



Certificate of Calibration

Equipment:	Hot Air Oven	Certificate No.:	C31241025
Model:	UFE 400	Issued Date:	17 May 2024
Serial No.(or ID):	G412.0022	Job No.:	WO-00027714
Manufacturer:	Memmert	Page:	1 of 5
Condition:	In Condition	Ventilation Valve:	Closed
Shelves(pc.):	1		

Customer: LIFE & ENVIRONMENT CO., LTD.
90, 92, 94 Soi On-nuch 64, Srinakarin Road, On-nuch,
Suanluang, Bangkok 10250 Thailand

Environment Condition:

Temperature:	27 °C	±	1.0 °C
Humidity:	56 %RH	±	5.7 %RH
Voltage:	230 VAC	±	2.1 VAC

Calibration Place: LIFE & ENVIRONMENT CO., LTD. (Water & Soil Testing Laboratory)
90, 92, 94 Soi On-nuch 64, Srinakarin Road, On-nuch,
Suanluang, Bangkok 10250 Thailand

Calibration By: Mr. Nakarin Ruenros
Calibration Date: 16 May 2024
The Method used: In house method, CAL-WI-16, base on TLAS-G20

Traceability: This certificate is traceable to the SI Units maintained by National Institute of Metrology (NIMT), Thailand through DKSH Technology Limited.
Certificate No. C10230023



Person in charge




Authorized signatory

This certificate is issued the units of measurement according to the International System of Units (SI). It provides traceability of measurement to international or national standard or other recognized national standard laboratories.

The measurement uncertainty stated is the expanded uncertainty which is obtained from the standard uncertainty multiplied by the coverage factor (k=2) to provide a level of confidence of approximately 95%. It is determined in accordance with the Guide to Expression of Uncertainty in Measurement (GUM).

These results may be affected by deviations from specified conditions. The results relate only to the items tested, calibrated or sampled. The report shall not be reproduced except in full without approval of DKSH Technology Limited.

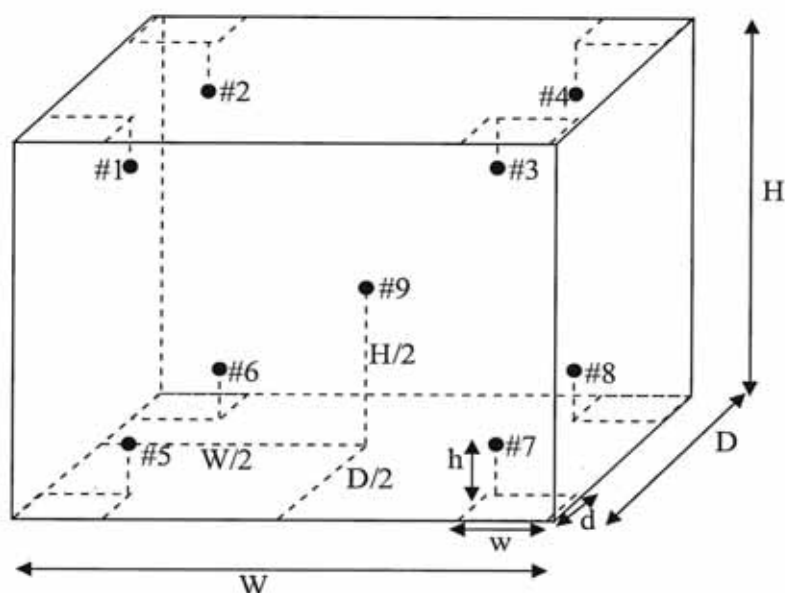

Standard Installation Locations

Volume (Calibration Zone)= 21 (Liters)

Inside chamber: $W = 40$ (cm) $D = 33$ (cm) $H = 40$ (cm)

Standard Locations (#1, #2, #3, #4): $w = 5$ (cm) $d = 5$ (cm) $h = 5$ (cm)

Standard Locations (#5, #6, #7, #8): $w = 5$ (cm) $d = 5$ (cm) $h = 5$ (cm)

#9: Geometric center of the chamber

Position of Std	#1	#2	#3	#4	#5	#6	#7	#8	#9
Channel of Logger	101	102	103	104	105	106	107	108	109

Definitions

Indicating Temperature: The average reading of indicating device which forms the integral part of the enclosure.

Measured Temperature: The average reading of standards at any positions or location.

Measured Uniformity: The maximum difference of measured temperatures between of any probes and the measured temperature at the reference location which are observed at same time or at close observation time as possible to determine the temperature pattern or homogeneity with the chamber at steady-state. The reference probe is preferably located in the geometric center of the chamber.

Measured Stability: The one-half of greatest maximum difference of measured temperatures at any one probe.

Overall Variation: The difference of maximum and minimum measured temperatures throughout observation time.

Calibration Results:

Without adjustment

Measurement Temperature at Spread Locations, Indicating of Unit Under Calibration: 104.0 °C

Locations	Measured Temperature (°C)	Correction of UUC. (°C)	Uncertainty (± °C)
#1	104.27	0.27	0.39
#2	104.30	0.30	0.39
#3	103.80	-0.20	0.39
#4	104.15	0.15	0.39
#5	104.26	0.26	0.39
#6	104.15	0.15	0.39
#7	103.79	-0.21	0.39
#8	103.98	-0.02	0.39
#9	104.33	0.33	0.39

Temperature Distribution

Desired (°C)	Setting (°C)	Indicating (°C)	Measured Temperature at Spread Locations (°C)									Uncertainty (± °C)*
			#1	#2	#3	#4	#5	#6	#7	#8	#9	
104.0	104.0	104.0	104.27	104.30	103.80	104.15	104.26	104.15	103.79	103.98	104.33	0.39

Chamber Characterization

Indicating (°C)	Measured Uniformity (°C)	Measured Stability (± °C)	Overall Variation (°C)
104.0	0.65	0.10	0.72

Note: * Maximum uncertainty of the each position

Without adjustment (Cont.)

Measurement Temperature at Spread Locations, Indicating of Unit Under Calibration: 150.0 °C

Locations	Measured Temperature (°C)	Correction of UUC. (°C)	Uncertainty (± °C)
#1	150.35	0.35	0.39
#2	150.43	0.43	0.39
#3	149.42	-0.58	0.39
#4	150.13	0.13	0.39
#5	150.51	0.51	0.39
#6	150.30	0.30	0.39
#7	149.56	-0.44	0.40
#8	150.00	0.00	0.39
#9	150.33	0.33	0.39

Temperature Distribution

Desired (°C)	Setting (°C)	Indicating (°C)	Measured Temperature at Spread Locations (°C)									Uncertainty (± °C)*
			#1	#2	#3	#4	#5	#6	#7	#8	#9	
150.0	150.0	150.0	150.35	150.43	149.42	150.13	150.51	150.30	149.56	150.00	150.33	0.40

Chamber Characterization

Indicating (°C)	Measured Uniformity (°C)	Measured Stability (± °C)	Overall Variation (°C)
150.0	0.99	0.09	1.21

Note: * Maximum uncertainty of the each position

Without adjustment (Cont.)

Measurement Temperature at Spread Locations, Indicating of Unit Under Calibration: 180.0 °C

Locations	Measured Temperature (°C)	Correction of UUC. (°C)	Uncertainty (± °C)
#1	180.31	0.31	0.49
#2	180.46	0.46	0.49
#3	179.05	-0.95	0.50
#4	179.99	-0.01	0.49
#5	180.71	0.71	0.49
#6	180.36	0.36	0.50
#7	179.39	-0.61	0.50
#8	180.02	0.02	0.49
#9	180.51	0.51	0.50

Temperature Distribution

Desired (°C)	Setting (°C)	Indicating (°C)	Measured Temperature at Spread Locations (°C)									Uncertainty (± °C)*
			#1	#2	#3	#4	#5	#6	#7	#8	#9	
180.0	180.0	180.0	180.31	180.46	179.05	179.99	180.71	180.36	179.39	180.02	180.51	0.50

Chamber Characterization

Indicating (°C)	Measured Uniformity (°C)	Measured Stability (± °C)	Overall Variation (°C)
180.0	1.65	0.11	1.83

Note: * Maximum uncertainty of the each position

The End of Certificate



Certificate of Calibration

Equipment:	Liquid Bath	Certificate No.:	C13230368
Model:	1013	Issued Date:	06 November 2023
Serial No. (or ID.):	10637804J (WM-WB-01/05)	Job No.:	WO-00008954
Manufacturer:	GFL	Page:	1 of 3
Condition:	In Condition		
Forced Circulation:	None		

Customer: LIFE & ENVIRONMENT CO., LTD.
90, 92, 94 Soi On-nuch 64, Srinakarin Road,
Suanluang, Bangkok 10250 Thailand

Environment Condition: Temperature: 24 °C ± 0.6 °C
Humidity: 50 %RH ± 4.4 %RH
Voltage: 224 VAC ± 2.5 VAC


Calibration Place: LIFE & ENVIRONMENT CO., LTD. (Microbiological Laboratory)
90, 92, 94 Soi On-nuch 64, Srinakarin Road,
Suanluang, Bangkok 10250 Thailand

Calibration By: Mr. Suphakorn Sookmee


Calibration Date: 06 November 2023

The Method used: In house method, CAL-WI-17, base on ASTM E715-80

Traceability: This certificate is traceable to the SI Units maintained by National Institute of Metrology (NIMT), Thailand through DKSH Technology Limited.
Certificate No. C10230019

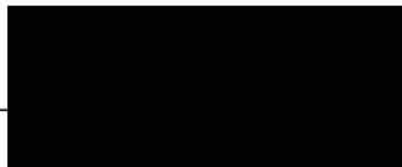

Person in charge

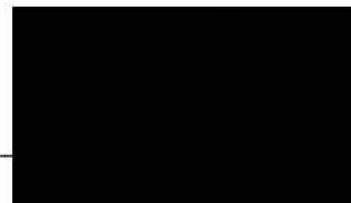


Authorized signatory

This certificate is issued the units of measurement according to the International System of Units (SI). It provides traceability of measurement to international or national standard or other recognized national standard laboratories.

The measurement uncertainty stated is the expanded uncertainty which is obtained from the standard uncertainty multiplied by the coverage factor ($k=2$) to provide a level of confidence of approximately 95%. It is determined in accordance with the Guide to Expression of Uncertainty in Measurement (GUM).

These results may be affected by deviations from specified conditions. The results relate only to the items tested, calibrated or sampled. The report shall not be reproduced except in full without approval of DKSH Technology Limited.

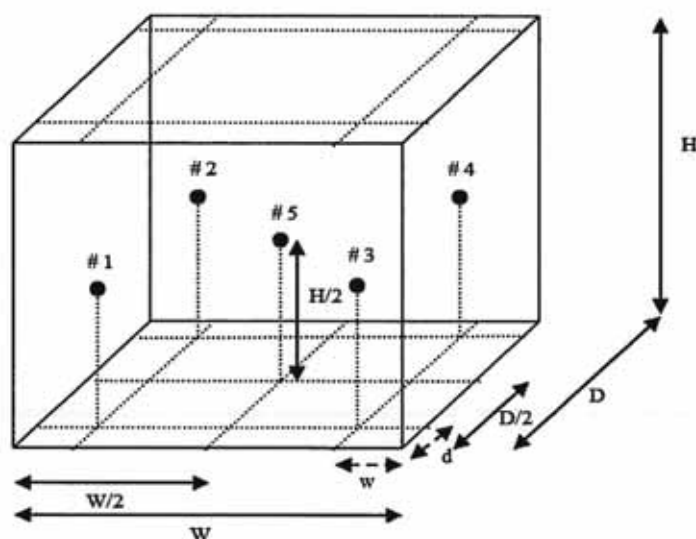

Standard Installation Locations

Midway between the diffuser plate and the water surface

Inside bath: W = 40 (cm) D = 25 (cm) H = 17 (cm) Volume = 17 (Liters)

Standard Locations #1: w = 5 (cm) d = 5 (cm)

Standard Locations #2: w = 5 (cm) d = 5 (cm)

Standard Locations #3: w = 5 (cm) d = 5 (cm)

Standard Locations #4: w = 5 (cm) d = 5 (cm)

Standard Locations #5: Center of any probes. (#1 - #4)

Position of Std	#1	#2	#3	#4	#5
Channel of Logger	301	302	303	304	309

Definitions

Indicating Temperature: The average reading of indicating device which forms the integral part of the bath.

Measured Temperature: The average reading of standards at any positions or location.

Measured Uniformity: The maximum difference of measured temperatures between of any probes and the measured temperature at the reference location which are observed at same time or at close observation time as possible to determine the temperature pattern or homogeneity with the bath at steady-state. The reference probe is preferably located in the geometric center of the bath.

Measured Stability: The one-half of greatest maximum difference of measured temperatures at any one probe.

Overall Variation: The difference of maximum and minimum measured temperatures throughout observation time.

Calibration Results:

Without adjustment

Measurement Temperature at Spread Locations, Indicating of Unit Under Calibration: 44.5 °C

Locations	Measured Temperature (°C)	Correction of UUC. (°C)	Uncertainty (\pm °C)
#1	44.50	0.00	0.15
#2	44.49	-0.01	0.16
#3	44.46	-0.04	0.15
#4	44.48	-0.02	0.15
#5	44.49	-0.01	0.15

Temperature Distribution

Desired (°C)	Setting (°C)	Indicating (°C)	Measured Temperature at Spread Locations (°C)					Uncertainty (\pm °C)*
			#1	#2	#3	#4	#5	
44.5	44.5	44.5	44.50	44.49	44.46	44.48	44.49	0.16

Bath Characterization

Indicating (°C)	Measured Uniformity (°C)	Measured Stability (\pm °C)	Overall Variation (°C)
44.5	0.04	0.03	0.07

Note: * Maximum uncertainty of the each position

The End of Certificate



Certificate of Calibration

Equipment:	Liquid Bath	Certificate No.:	C13240371
Model:	1013	Issued Date:	08 November 2024
Serial No. (or ID.):	10637804J (WM-WB-01/05)	Job No.:	WO-00047861
Manufacturer:	GFL	Page:	1 of 3
Condition:	In Condition		
Forced Circulation:	None		

Customer: LIFE & ENVIRONMENT CO., LTD.
90, 92, 94 Soi On-nuch 64, Srinakarin Road, On-nuch,
Suanluang, Bangkok 10250 Thailand

Environment Condition: Temperature: 25 °C \pm 1.3 °C
Humidity: 51 %RH \pm 5.2 %RH
Voltage: 229 VAC \pm 2.0 VAC


Calibration Place: LIFE & ENVIRONMENT CO., LTD. (Microbiological Laboratory)
90, 92, 94 Soi On-nuch 64, Srinakarin Road, On-nuch,
Suanluang, Bangkok 10250 Thailand

Calibration By: Mr. Suphanimit Khamnonphoem

Calibration Date: 05 November 2024

The Method used: In house method, CAL-WI-17, base on ASTM E715-80

Traceability: This certificate is traceable to the SI Units maintained by National Institute of Metrology (NIMT), Thailand through DKSH Technology Limited.
Certificate No. C10240005

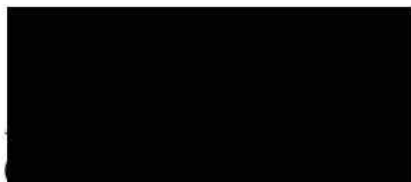

Person in charge




Authorized signatory

This certificate is issued the units of measurement according to the International System of Units (SI). It provides traceability of measurement to international or national standard or other recognized national standard laboratories.

The measurement uncertainty stated is the expanded uncertainty which is obtained from the standard uncertainty multiplied by the coverage factor ($k=2$) to provide a level of confidence of approximately 95%. It is determined in accordance with the Guide to Expression of Uncertainty in Measurement (GUM).

These results may be affected by deviations from specified conditions. The results relate only to the items tested, calibrated or sampled. The report shall not be reproduced except in full without approval of DKSH Technology Limited.

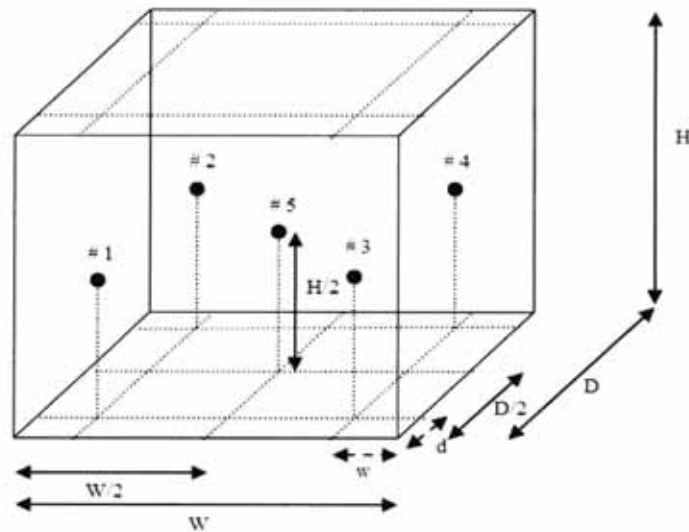

Standard Installation Locations

Midway between the diffuser plate and the water surface

Inside bath: W = 40 (cm)	D = 25 (cm)	H = 17 (cm)	Volume = 17 (Liters)
Standard Locations #1:	w = 5 (cm)	d = 5 (cm)	
Standard Locations #2:	w = 5 (cm)	d = 5 (cm)	
Standard Locations #3:	w = 5 (cm)	d = 5 (cm)	
Standard Locations #4:	w = 5 (cm)	d = 5 (cm)	

Standard Locations #5: Center of any probes. (#1 - #4)

Position of Std	#1	#2	#3	#4	#5
Channel of Logger	301	302	303	304	305

Definitions

Indicating Temperature: The average reading of indicating device which forms the integral part of the bath.

Measured Temperature: The average reading of standards at any positions or location.

Measured Uniformity: The maximum difference of measured temperatures between of any probes and the measured temperature at the reference location which are observed at same time or at close observation time as possible to determine the temperature pattern or homogeneity with the bath at steady-state. The reference probe is preferably located in the geometric center of the bath.

Measured Stability: The one-half of greatest maximum difference of measured temperatures at any one probe.

Overall Variation: The difference of maximum and minimum measured temperatures throughout observation time.

Calibration Results:

Without adjustment

Measurement Temperature at Spread Locations, Indicating of Unit Under Calibration: 44.5 °C

Locations	Measured Temperature (°C)	Correction of UUC. (°C)	Uncertainty (± °C)
#1	44.39	-0.11	0.15
#2	44.48	-0.02	0.15
#3	44.43	-0.07	0.15
#4	44.34	-0.16	0.15
#5	44.40	-0.10	0.16

Temperature Distribution

Desired (°C)	Setting (°C)	Indicating (°C)	Measured Temperature at Spread Locations (°C)					Uncertainty (± °C)*
			#1	#2	#3	#4	#5	
44.5	44.5	44.5	44.39	44.48	44.43	44.34	44.40	0.16

Bath Characterization

Indicating (°C)	Measured Uniformity (°C)	Measured Stability (± °C)	Overall Variation (°C)
44.5	0.12	0.03	0.16

Note: * Maximum uncertainty of the each position

The End of Certificate



Certificate of Calibration

Equipment:	Autoclave	Certificate No.:	C11230236
Model:	88	Issued Date:	13 December 2023
Serial No. (or ID.):	105611	Job No.:	WO-00011851
Manufacturer:	ALP	Page:	1 of 3
Condition:	In Condition		

Customer: LIFE & ENVIRONMENT CO., LTD.
90, 92, 94 Soi On-nuch 64, Srinakarin Road,
On-nuch, Suanluang, Bangkok 10250 Thailand.

Environment Condition: Temperature: 26 °C ± 0.6 °C
Humidity: 51 %RH ± 4.0 %RH
Voltage: 226 VAC ± 1.5 VAC

Calibration Place: LIFE & ENVIRONMENT CO., LTD. (Microbiogy Testing Laboratory)
90, 92, 94 Soi On-nuch 64, Srinakarin Road,
On-nuch, Suanluang, Bangkok 10250 Thailand.

Calibration By: Mr. Siwapan Srijan

Calibration Date: 13 December 2023

The Method used: In house method, CAL-WI-18, base on BS 2646 : Part 5

Traceability: This certificate is traceable to the SI Units maintained by National Institute of Metrology (NIMT), Thailand through Quality reborn Co., Ltd.
Certificate No.QR23-0487



Person in charge




Authorized signatory

This certificate is issued the units of measurement according to the International System of Units (SI). It provides traceability of measurement to international or national standard or other recognized national standard laboratories.

The measurement uncertainty stated is the expanded uncertainty which is obtained from the standard uncertainty multiplied by the coverage factor (k=2) to provide a level of confidence of approximately 95%. It is determined in accordance with the Guide to Expression of Uncertainty in Measurement (GUM).

These results may be affected by deviations from specified conditions. The results relate only to the items tested, calibrated or sampled. The report shall not be reproduced except in full without approval of DKSH Technology Limited.

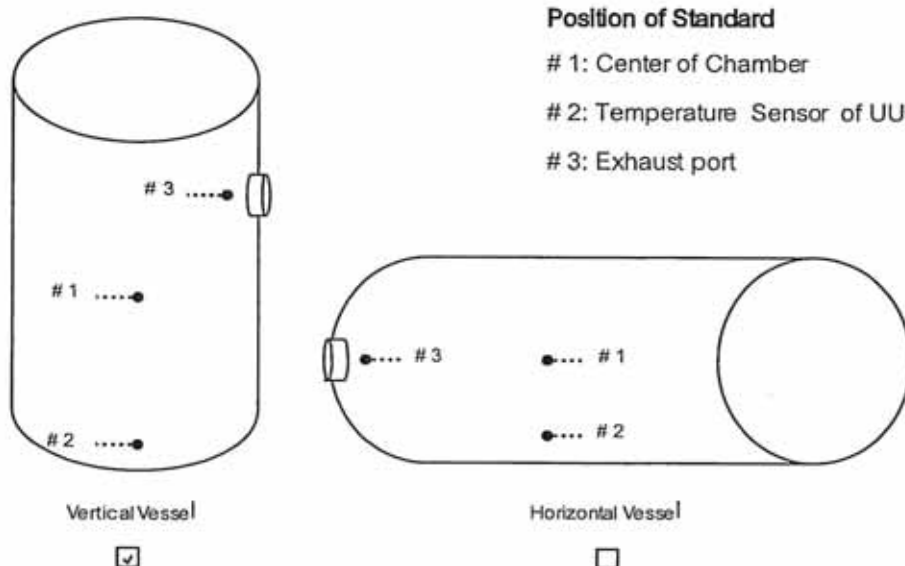

Standard Installation Locations

- Standard Locations (#1): Geometric center of the chamber
- Standard Locations (#2): Distance from temperature sensor of UUC 2 (cm.)
- Standard Locations (#3): Distance from the wall 5 (cm.)

Position of Std	#1	#2	#3
Channel of Logger	10	11	12

Definitions

Indicating Temperature: The average reading of indicating device which forms the integral part of the enclosure.

Measured Temperature: The average reading of standards at any positions or location.

Measured Stability: The one-half of greatest maximum difference of measured temperatures at any one probe.

Calibration Results:

Without adjustment

Measurement Temperature at Spread Locations, Indicating of Unit Under Calibration: 121 °C

Locations	Measured Temperature (°C)	Correction of UUC. (°C)	Uncertainty (± °C)
#1	121.02	0.02	1.8
#2	121.02	0.02	1.9
#3	121.05	0.05	2.0

Temperature Distribution

Temperature			Pressure	Measured Temperature at Spread Locations			Uncertainty (± °C)*
Desired (°C)	Setting (°C)	Indicating (°C)	Indicating kg/cm ²	#1 (°C)	#2 (°C)	#3 (°C)	
121	121	121	1.2	121.02	121.02	121.05	2.0

Chamber Characterization

Indicating Temperature (°C)	Indicating Pressure kg/cm ²	Measured Stability (± °C)
121	1.2	1.63

Note: * Maximum uncertainty of the each position

Record every 10 seconds after reaching steady state or after one achieved complete cycle.

The End of Certificate



Certificate of Calibration

Equipment:	Autoclave	Certificate No.:	C11240219
Model:	88	Issued Date:	13 December 2024
Serial No. (or ID.):	105611	Job No.:	WO-00054728
Manufacturer:	ALP	Page:	1 of 3
Condition:	In Condition		

Customer: LIFE & ENVIRONMENT CO., LTD.
90, 92, 94 Soi On-nuch 64, Srinakarin Road, On-nuch,
Suanluang, Bangkok 10250 Thailand

Environment Condition: Temperature: 27 °C ± 0.5 °C
Humidity: 53 %RH ± 3.1 %RH
Voltage: 227 VAC ± 3.6 VAC

Calibration Place: LIFE & ENVIRONMENT CO., LTD. (Microbiology Testing Laboratory)
90, 92, 94 Soi On-nuch 64, Srinakarin Road, On-nuch,
Suanluang, Bangkok 10250 Thailand

Calibration By: Mr. Piyapat Saidoung


Calibration Date: 12 December 2024

The Method used: In house method, CAL-WI-18, base on BS 2646 : Part 5

Traceability: This certificate is traceable to the SI Units maintained by National Institute of Metrology (NIMT), Thailand through Quality reborn Co., Ltd.
Certificate No.QR24-0463



Person in charge

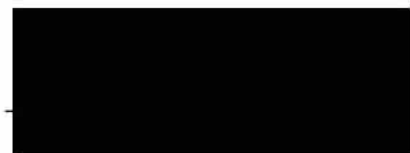

Authorized signatory

This certificate is issued the units of measurement according to the International System of Units (S). It provides traceability of measurement to international or national standard or other recognized national standard laboratories.

The measurement uncertainty stated is the expanded uncertainty which is obtained from the standard uncertainty multiplied by the coverage factor ($k=2$) to provide a level of confidence of approximately 95%. It is determined in accordance with the Guide to Expression of Uncertainty in Measurement (GUM).


These results may be affected by deviations from specified conditions. The results relate only to the items tested, calibrated or sampled. The report shall not be reproduced except in full without approval of DKSH Technology Limited.

Position of Standards

1: Upper haft of the chamber

2: Temperature sensor of UUC

3: Exhaust port

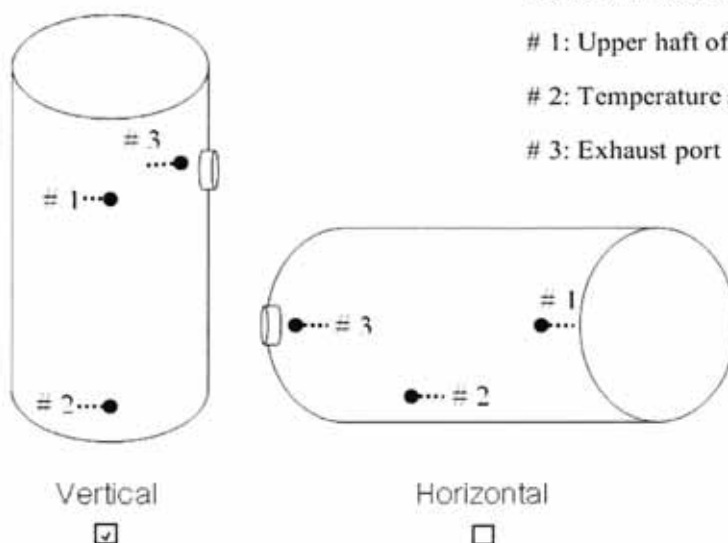

Standard Installation Locations

Standard Locations (#1): Geometric center of the chamber

Standard Locations (#2): Distance from temperature sensor of UUC 2 (cm.)

Standard Locations (#3): Distance from the wall 5 (cm.)

Position of Std	#1	#2	#3
Channel of Logger	10	11	12

Definitions

Indicating Temperature: The average reading of indicating device which forms the integral part of the enclosure.

Measured Temperature: The average reading of standards at any positions or location.

Measured Stability: The one-half of greatest maximum difference of measured temperatures at any one probe.

Calibration Results:
Without adjustment

Measurement Temperature at Spread Locations, Indicating of Unit Under Calibration: 121 °C

Locations	Measured Temperature (°C)	Correction of UUC. (°C)	Uncertainty (± °C)
#1	121.14	0.14	2.1
#2	121.20	0.20	2.0
#3	121.15	0.15	1.9

Temperature Distribution

Temperature			Pressure	Measured Temperature at Spread Locations			Uncertainty (± °C)*
Desired (°C)	Setting (°C)	Indicating (°C)	Indicating kg/cm ²	#1 (°C)	#2 (°C)	#3 (°C)	
121	121	121	1.2	121.14	121.20	121.15	2.1

Chamber Characterization

Indicating Temperature (°C)	Indicating Pressure kg/cm ²	Measured Stability (± °C)
121	1.2	1.69

Note: * Maximum uncertainty of the each position

Record every 10 seconds after reaching steady state or after one achieved complete cycle.

The End of Certificate




Calibration Test Report

Calibrated at : บริษัท ไทยชินก อินดัสตรี คอร์ปอเรชั่น จำกัด
Reference Standard : Sound Calibrator Class 1 Model QC-10
 Serial No.QIG030022
 Date of Calibration : 07/5/2024

Date	Serial No.	Reference Standard (dB)	Instrument Reading (dB)	Adjust	Error (dB)	After Use	Error (dB)	Inspection Result	Calibrated By
19/7/2567	112033	114.0	114.0	114.0	0.0	114.0	0.0	Pass	พิทักษ์ธรรม ต.
19/7/2567	820752	114.0	114.0	114.0	0.0	114.0	0.0	Pass	พิทักษ์ธรรม ต.
19/7/2567	820755	114.0	114.0	114.0	0.0	114.0	0.0	Pass	พิทักษ์ธรรม ต.
19/7/2567	820756	114.0	114.0	114.0	0.0	114.0	0.0	Pass	พิทักษ์ธรรม ต.

หมายเหตุ : Error \pm 1.5 dB

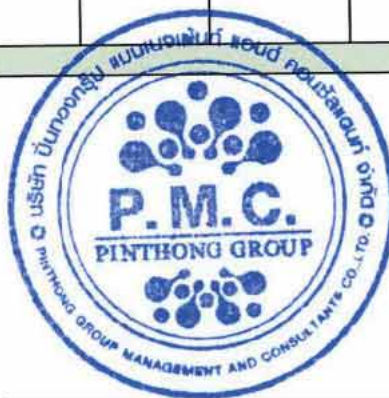

Approve By : _____

Date :19../...ค.ค../...2567...

Certificate of Calibration

Certificate No. : WK2405-033-1

Page 1 of 2

Customer : Pinthong Group Management and Consultants Co.,Ltd.
27 Rama 2 Road, Thakham,
Bangkuntien, Bangkok, 10150, Thailand.

Instrument	: Calibrator	Ambient Temperature	: (23 ± 2)°C
Manufacturer	: Quest Technologies	Humidity	: (50 ± 15) %RH
Model	: QC-10	Received Date	: 3-May-24
Serial No.	: QIG030022	Calibrated Date	: 7-May-24
Identity No.	: N/A	Issued Date	: 8-May-24
Range	: See to Data	Calibrated Location	: In Lab
Resolution	: See to Data		

Calibration Method : CP-WK-A02, CP-WK-TF03, CP-WK-E19

Reference Standard Instruments :

Instrument	Serial No.	Certificate No.	Due Date	Traceability to
Data Acquisition/Switch Unit	MY41011202	WK2401-049-1	5-Jan-25	WK Electric Co., Ltd
Sound Level Calibrator	10049416	EELBP.196/0166	27-Jan-25	TISTR
Universal Counter	3416A08501	TTH-0-89055	19-Feb-26	Technmaster
Audio Analyzer	3413A14479	E3U2400174	13-Feb-26	NA

TISTR : Thailand Institute of Scientific and Technological Research.
Technmaster : Technmaster Asia (Thailand) Co., Ltd.
NA : NA Caltechnologies, Ltd.

This result calibrate was found accurate as shown on date place of calibrate only
This certificate is traceability to the International System of Unit (SI)

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence approximately 95 %

Calibrated by :

Approved by :

Authorized Signatory



Calibration Results

Certificate No.: WK2405-033-1

Page 2 of 2

Calibration Results

Function : Sound Level Pressure Measurement @ 1kHz

Nominal Value (dB)	STD Value (dB)	Error (dB)	(±) Uncertainty (dB)
94	113.97	0.03	0.061

Function : Frequency Measurement

Nominal Value (Hz)	STD Value (Hz)	Error (Hz)	(±) Uncertainty (Hz)
1000	1000.023	-0.023	0.58

(X) Without Adjustment () After Adjustment

This certificate may not be reproduced except in full unless permission for the reproduction has been obtained in writing from the laboratory.

**** End of Certificate****

Certificate of Calibration

Certificate No.: WK2403-103-2 Page 1 of 2

Customer : PINTHONG GROUP MANAGEMENT AND CONSULTANTS CO., LTD.
27 Rama 2 Road, Thakham, Bangkokkuen,
Bangkok 10150 Thailand

Instrument	: Sound Level Meter	Ambient Temperature	: (23 ± 2) °C
Manufacturer	: N/A	Humidity	: (50 ± 15) %RH
Model	: TYPE 6236	Received Date	: 11-Mar-24
Serial No.	: 112033	Calibrated Date	: 12-Mar-24
Identity No.	: N/A	Issued Date	: 18-Mar-24
Range	: See to Data	Calibrated Location	: In Lab
Resolution	: 0.1 dB		
Calibration Method	: CP-WK-A01		

Reference standard instruments :

Instrument	Serial No.	Certificate No.	Due Date	Traceability to
Sound Level Calibrator	10049416	EEL.BP. 196/0166	27-Jan-25	TISTR

TISTR : Thailand Institute of Scientific and Technological Research.
This result calibrate was found accurate as shown on date place of calibrate only
This certificate is traceability to the International System of Unit (SI)

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k=2, providing a level of confidence approximately 95%

Calibrated by :

Approved by :

Authorized Signatory

This certificate may not be reproduced except in full unless permission for the reproduction has been obtained in writing from the laboratory.

Calibration Results

Certificate No.: WK2403-103-2 Page 2 of 2

Calibration Result of the Accuracy

Function : Sound Level Measurement at 1 kHz

Range : A Mode : Fast Resolution : 0.1 dB

STD Setting	UUC Reading	Error	Uncertainty (± dB)
94	94.0	0.0	0.20
114	114.2	0.2	0.20

Range : A Mode : Slow Resolution : 0.1 dB

STD Setting	UUC Reading	Error	Uncertainty (± dB)
94	93.9	-0.1	0.20
114	114.2	0.2	0.20

Range : C Mode : Fast Resolution : 0.1 dB

STD Setting	UUC Reading	Error	Uncertainty (± dB)
94	94.0	0.0	0.20
114	114.2	0.2	0.20

Range : C Mode : Slow Resolution : 0.1 dB

STD Setting	UUC Reading	Error	Uncertainty (± dB)
94	93.9	-0.1	0.20
114	114.2	0.2	0.20

(X) Without Adjustment () After Adjustment

This certificate may not be reproduced except in full unless permission for the reproduction has been obtained in writing from the laboratory.
**** End of Certificate ****

Certificate of Calibration

Certificate No.: WK2405-033-2

Page 1 of 2

Customer : Pinthong Group Management and Consultants Co.,Ltd.
27 Rama 2 Road, Thakham,
Bangkuntien, Bangkok, 10150, Thailand.

Instrument : Sound Level Meter	Ambient Temperature : (23 ± 2) °C
Manufacturer : Scarlet Tech	Humidity : (50 ± 15) %RH
Model : ST 21D	Received Date : 3-May-24
Serial No. : 820752	Calibrated Date : 7-May-24
Identity No. : N/A	Issued Date : 8-May-24
Range : See to Data	Calibrated Location : In Lab
Resolution : 0.1 dB	

Calibration Method : CP-WK-A01

Reference standard instruments :

Instrument	Serial No.	Certificate No.	Due Date	Traceability to
Sound Level Calibrator	10049416	EEL.BP. 196/0166	27-Jan-25	TISTTR

TISTTR : Thailand Institute of Scientific and Technological Research.
This result calibrate was found accurate as shown on date place of calibrate only
This certificate is traceability to the International System of Unit (SI)

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k=2, providing a level of confidence approximately 95%

Calibrated by :
Approved by :

Authorized Signatory

This certificate may not be reproduced except in full unless permission for the reproduction has been obtained in writing from the laboratory.

Calibration Results

Certificate No. : WK2405-033-2

Page 2 of 2

Calibration Result of the Accuracy
Function : Sound Level Measurement at 1 kHz

Range : A	Mode : Fast	Resolution : 0.1 dB	STD Setting	UUC Reading	Error	Uncertainty (± dB)
			94	94.0	0.0	0.20
			114	113.9	-0.1	0.20

Range : A	Mode : Slow	Resolution : 0.1 dB	STD Setting	UUC Reading	Error	Uncertainty (± dB)
			94	94.0	0.0	0.20
			114	113.9	-0.1	0.20

Range : C	Mode : Fast	Resolution : 0.1 dB	STD Setting	UUC Reading	Error	Uncertainty (± dB)
			94	94.0	0.0	0.20
			114	113.9	-0.1	0.20

Range : C	Mode : Slow	Resolution : 0.1 dB	STD Setting	UUC Reading	Error	Uncertainty (± dB)
			94	94.0	0.0	0.20
			114	113.9	-0.1	0.20

(X) Without Adjustment () After Adjustment

This certificate may not be reproduced except in full unless permission for the reproduction has been obtained in writing from the laboratory.

**** End of Certificate ****

Certificate of Calibration

Certificate No.: WK2405-033-4

Customer : Pinhong Group Management and Consultants Co., Ltd.
 27 Rama 2 Road, Thakham,
 Bangkuntien, Bangkok, 10150, Thailand.

Instrument : Sound Level Meter
 Manufacturer : Scalet Tech
 Model : ST 21D
 Serial No. : 820755
 Identity No. : N/A
 Range : See to Data
 Resolution : 0.1 dB
 Ambient Temperature : (23 ± 2) °C
 Humidity : (50 ± 15)%RH
 Received Date : 3-May-24
 Calibrated Date : 7-May-24
 Issued Date : 8-May-24
 Calibrated Location : In Lab

Calibration Method : CP-WK-A01

Reference standard instruments :

Instrument	Serial No.	Certificate No.	Due Date	Traceability to
Sound Level Calibrator	10049416	EEL.BP.196/0166	27-Jan-25	TISTR

TISTR : Thailand Institute of Scientific and Technological Research.
 This result calibrate was found accurate as shown on date place of calibrate only
 This certificate is traceability to the International System of Unit (SI)

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k=2, providing a level of confidence approximately 95%

Calibrated by :

Approved by :

Authorized Signatory

This certificate may not be reproduced except in full unless permission for the reproduction has been obtained in writing from the laboratory.

Calibration Results

Certificate No. : WK2405-033-4

Calibration Result of the Accuracy

Function : Sound Level Measurement at 1 kHz

Range : A Mode : Fast Resolution : 0.1 dB

STD Setting	UUC Reading	Error	Uncertainty (± dB)
94	94.0	0.0	0.20
114	114.1	0.1	0.20

Range : A Mode : Slow Resolution : 0.1 dB

STD Setting	UUC Reading	Error	Uncertainty (± dB)
94	94.0	0.0	0.20
114	114.1	0.1	0.20

Range : C Mode : Fast Resolution : 0.1 dB

STD Setting	UUC Reading	Error	Uncertainty (± dB)
94	94.0	0.0	0.20
114	114.0	0.0	0.20

Range : C Mode : Slow Resolution : 0.1 dB

STD Setting	UUC Reading	Error	Uncertainty (± dB)
94	94.0	0.0	0.20
114	114.0	0.0	0.20

(X) Without Adjustment () After Adjustment

This certificate may not be reproduced except in full unless permission for the reproduction has been obtained in writing from the laboratory.
 ***** End of Certificate *****



Certificate of Calibration

Certificate No.: WK2405-033-5

Page 1 of 2

Customer : Pinthong Group Management and Consultants Co.,Ltd.
27 Rama 2 Road, Thakham,
Bangkuntien, Bangkok, 10150, Thailand.

Instrument : Sound Level Meter	Ambient Temperature : (23 ± 2) °C
Manufacturer : Scarlet Tech	Humidity : (50 ± 15)%RH
Model : ST 21D	Received Date : 3-May-24
Serial No. : 820756	Calibrated Date : 7-May-24
Identity No. : N/A	Issued Date : 8-May-24
Range : See to Data	Calibrated Location : In Lab
Resolution : 0.1 dB	

Calibration Method : CP-WK-A01

Reference standard instruments :

Instrument	Serial No.	Certificate No.	Due Date	Traceability to
Sound Level Calibrator	100-9416	EEL.BP. 196/0166	27-Jan-25	TISTR

TISTR : Thailand Institute of Scientific and Technological Research.
This result calibrate was found accurate as shown on date place of calibrate only
This certificate is traceability to the International System of Unit (SI)

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k=2, providing a level of confidence approximately 95%

Calibrated by :

Approved by :

Authorized Signatory

This certificate may not be reproduced except in full unless permission for the reproduction has been obtained in writing from the laboratory.

Calibration Results

Certificate No. : WK2405-033-5

Page 2 of 2

Calibration Result of the Accuracy

Function : Sound Level Measurement at 1 kHz

Range : A Mode : Fast Resolution : 0.1 dB

STD Setting	UUC Reading	Error	Uncertainty (± dB)
94	94.0	0.0	0.20
114	114.0	0.0	0.20

Range : A Mode : Slow Resolution : 0.1 dB

STD Setting	UUC Reading	Error	Uncertainty (± dB)
94	94.0	0.0	0.20
114	114.0	0.0	0.20

Range : C

Mode : Fast Resolution : 0.1 dB

STD Setting	UUC Reading	Error	Uncertainty (± dB)
94	94.0	0.0	0.20
114	113.9	-0.1	0.20

Range : C

Mode : Slow Resolution : 0.1 dB

STD Setting	UUC Reading	Error	Uncertainty (± dB)
94	94.0	0.0	0.20
114	113.9	-0.1	0.20

(X) Without Adjustment () After Adjustment

This certificate may not be reproduced except in full unless permission for the reproduction has been obtained in writing from the laboratory.

**** End of Certificate ****



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG, BANGKOK 10250
TEL. 0-2717-3000-24 FAX. 0-2719-9484



Certificate of Calibration

Certificate No. : 23E3924

Page : 1 of 2

Equipment : pH Meter
Manufacturer: Mettler Toledo
Model : SevenExcellence
Serial No.: B834291445
ID No.: RYG_EN0152
Condition As-Received: Used Item
Received Date: 08 December 2023
Calibration Date: 14 December 2023

This certificate may not be reproduced other than in full,
except with the prior written approval of the head of
Corporate Services 3: Equipment Calibration and Testing Services.

Reference: 2312-0151DSC
Ambient Temperature: (23 \pm 2) °C
Relative Humidity: (50 \pm 10) %

Submitted by: ALS Laboratory Group (Thailand) Co.,Ltd. Rayong Branch

616/10 Moo 5, T.Maenam Khu, A.Pluakdaeng,
Rayong 21140, Thailand

Procedure used: Calibration were conducted using calibration procedure No. CP-E17 according to EURAMET cg-15.

Condition of this result of calibration

1.Reference standards instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Certificate No.</u>	<u>Due Date</u>
1) Multi-Product Calibrator	5502A	2435802	EE-0041-23	26 Apr 2024

2.This result of calibration was made on requested at the point specified by customer.


3.The certificate is valid only to the item calibrated on date and place of calibration.

4.This Certification is traceable to the International System of Unit maintained through:-

-National Institute of Metrology Thailand (NIMT)

Calibrated by : Napachanok Prasomsoosiri
Issue Date : 15 December 2023

Approved Signatory



B 0331106



Cert. No.: 23E3924

Page.: 2 of 2

Result of calibration :- (*) Without adjustment () After adjustment

Function: DC voltage measurement

Range:

2000

mV

<u>Standard Value</u>	<u>UUC* Reading</u>	<u>Error</u>	<u>Uncertainty</u>
(mV)	(mV)	(mV)	($\pm \mu V$)
-200.0000	-199.9	0.1	68
-150.0000	-150.0	0.0	65
-100.0000	-100.0	0.0	63
-50.0000	-50.0	0.0	61
0.0000	0.0	0.0	58
50.0000	50.0	0.0	61
100.0000	100.0	0.0	63
150.0000	150.0	0.0	65
200.0000	199.9	-0.1	68

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k=2$, providing a level of confidence of approximately 95 %

UUC*= Unit Under Calibration.

-o0o-

a 1193422



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000-29 FAX. 0-2719-9484



Cert.No.: 23CH1574
Page.: 1 of 3

Certificate of Calibration

Equipment :	pH Meter
Manufacturer :	Mettler Toledo
Model :	SevenExcellence
Serial No. :	B834291445
ID No. :	RYG_EN0152
Condition As-Received:	Used Item
Received Date :	08 December 2023
Calibration Date :	15 December 2023
Reference :	2312-0151DSC-3
Submitted by :	ALS Laboratory Group (Thailand) Co.,Ltd. Rayong Branch 616/10 Moo 5, T.Maenam Khu, A.Pluakdaeng, Rayong 21140, Thailand
Ambient Temperature :	(25 ± 2.5) °C
Relative Humidity :	(50 ± 15) %
Calibration Procedure :	In - house method : - CP-CH5 by direct measurement with standard voltage calibrator and direct measurement with certified reference material (CRM) - CP-CH8 by comparison with standard thermometer

Calibrated by :

Approved by :

Issue Date :

19 December 2023

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

A 0061696



Cert.No.: 23CH1574

Page.: 2 of 3

Condition of this calibration result

1. Reference Standard Instrument : -

<u>Instrument</u>	<u>Serial No.</u>	<u>ID No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
1) Document Process Calibrator	54030049	130RC116	23E2802	27 Aug 2024
2) Ref. Standard Thermometer	4982054	110RC044	23I908	26 July 2024

This certification is traceable to the International System of Unit maintained through:-

- Technology Promotion Association (Thailand-Japan)

2. Certified Reference Materials : The measurement results are traceable to SI through CPA chem Ltd.,
ANSI-ASQ National Accreditation Board, Accredited No. AR-1835

<u>Buffer Solution</u>	<u>Manufacturer</u>	<u>Lot No.</u>	<u>Exp. date</u>
pH 4.008	CPA chem	913598	14 July 2025
pH 6.986	CPA chem	931959	01 Oct 2024
pH 9.997	CPA chem	940106	02 Nov 2024

3. This certificate is valid only to the item calibrated on date and place of calibration.

Calibration Results

Function : mV Measurement

Performing standard curve by Fluke at pH (4,7,10)

Unit Under Calibration	Nominal Value	Standard Voltage Input	Actual Reading		Uncertainty of Measurement (±mV)	Coverage factor <i>k</i>
	pH	mV	mV	pH		
pH Meter S/N.: B834291445	4.000	177.48	177.3	4.000	0.058	2.00
	7.000	0.00	-0.1	7.000	0.058	2.00
	10.000	-177.48	-177.5	10.000	0.058	2.00



a 1193852



Cert.No.: 23CH1574

Page.: 3 of 3

Calibration Results**Function : pH Measurement**

Performing three buffers standard curve by using buffer nominal pH (4,7,10)

Unit Under Calibration	Standard pH Buffer Solution	Actual pH Reading	Actual mV Reading (mV)	Uncertainty of pH measurement (\pm)	Coverage factor k
pH Electrode S/N.: 3225368	4.008	4.013	184.1	0.0045	2.00
	6.986	6.998	8.7	0.0084	2.00
	9.997	10.002	-164.7	0.0088	2.11

Function : Temperature Measurement**(*) Without adjustment**

This equipment was connected with Temperature Probe;

- Model : InLab®Expert Pro-ISM

- Serial No. : 3225368

Dimension of probe;

- Length : 120 mm

- Diameter : 12 mm

- Immersion Depth : 100 mm

Calibration Point (°C)	Standard Temperature (°C)	UUC* Reading (°C)	Error (°C)	Uncertainty of measurement (\pm °C)	Coverage factor k
25.0	25.003	24.3	-0.703	0.13	2.00

Remark : - UUC* = Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k , providing a level of confidence of approximately 95 %.

-o0o-



a 1193851

Certificate of System Qualification

GC-OQ + GCMS-OQ

REVIEW BY

APPROVED

NEXT CAL. DATE 13-Jun-25

System ID: GM-7
Organization Name: ALS Laboratory Group (Thailand) Co., Ltd.
Organization Location: 104 Patthanakarn 40, Patthanakarn Rd., Khwang Suan Luang, Khet Suan Luang, Bangkok.

Date: December 13, 2023 3:32:46 PM
EQP Name: AgilentRecommended , AgilentRecommended
EQP Revision: GC.02.50, GCMS.02.50
Overall Qualification Status: Pass

System Inspection and Basic Safety and Operation

Name: 7890
Setpoint Status: Pass

Overall System Inspection and Basic Safety and Operation Test Status
Pass

Inlet Pressure Accuracy

Name: 7890
Front SSL
Setpoint Status: Pass

	Setpoint		Actual	
Inlet Pressure:	25.0	psi	25.0	psi
Accuracy:			0.0	psi
Agilent Recommended:			<=	1.2

Overall Inlet Pressure Accuracy Test Status
Pass

GC Oven Temperature Accuracy

Name: 7890

Setpoint Status: Pass

Zone: Oven

Setpoint/Actual

Temperature: 230.0 232.3 °C

Accuracy: 2.3 °C

Agilent Recommended: >= -1.0 % setpoint in K (-5.0 °C)
<= 1.0 % setpoint in K (5.0 °C)

Setpoint Status: Pass

Zone: Oven

Setpoint/Actual

Temperature: 100.0 100.7 °C

Accuracy: 0.7 °C

Agilent Recommended: >= -1.0 % setpoint in K (-3.7 °C)
<= 1.0 % setpoint in K (3.7 °C)

Overall GC Oven Temperature Accuracy Test Status

Pass

GC Oven Temperature Stability

Name: 7890

Setpoint Status: Pass

Setpoint/Average

Temperature: 100.0 100.4 °C

Stability: 0.0 °C

Agilent Recommended: <= 0.5

Overall GC Oven Temperature Stability Test Status

Pass

Log Amp

Tested Combination1 Front SSL / External SQ

Name: 5977A

Setpoint Status: Pass

Date: December 13, 2023 3:32:46 PM

System ID: GM-7

Overall Log Amp Test Status

Pass

RFPA

Tested Combination1 Front SSL / External SQ

Name: 5977A

Setpoint Status: Pass

Amu: 1050 m/z Drift After Five Minutes: RFP Voltage: 504 mV

2 mV

Agilent Recommended: >= -100 and <= 100 <= 1100

Overall RFPA Test Status

Pass

Tune EI

Tested Combination1 Front SSL / External SQ

Name: 5977A

Setpoint Status: Pass

Filament: 1

Setpoint Status: Pass

Filament: 2

Overall Tune EI Test Status

Pass

Signal to Noise EI

Tested Combination1 Front SSL / External SQ

Name: 5977A

Source: EI - Extractor Filament: 1

Setpoint Status: Pass

Signal to Noise: 11318

Agilent Recommended: >= 1200

Source: EI - Extractor Filament: 2

Setpoint Status: Pass

Signal to Noise: 16588

Agilent Recommended: >= 1200

Overall Signal to Noise EI Test Status

Pass

NOTE: This test's 0 comment(s) and 6 deviation(s) are available in the Attachments section.

Instrument Details

Purpose

This section describes the as found system configuration.

Details

System

System ID	GM-7
Manufacturer	Agilent Technologies
Name	7890

Tested Combination1

Injection Technique	Manual Injection
Inlet	Front
Detector	External
LTM Included?	No

Sampler 1

Manufacturer	Agilent Technologies
Type	Manual Injection
Usage	Sample Injection
Syringe Volume (µL)	10

Mainframe 1

Manufacturer	Agilent Technologies
Name	7890
Model Number	G3442B
Serial Number	CN14133181
Firmware Revision	B.02.03
Oven Type	Standard

Inlet 1

Manufacturer	Agilent Technologies
Name	7890
Type	SSL
Location	Front
Carrier Gas	Helium
Control Type	Electronic Pressure Control (EPC)
Purged Inlet	Yes

Detector 1

Manufacturer	Agilent Technologies
Name	Mass Spectrometer
Type	Mass Spectrometer
Location	External

Mass Spectrometer 1

Manufacturer	Agilent Technologies
Type	SQ
Name	5977A
Serial Number	US1415M209
Firmware Revision	5977 6.00.21
High Vacuum System	Turbo Pump
Scouting Run Standard	OFN Std

MS EI Source 1

Manufacturer	Agilent Technologies
Source Type	EI - Extractor
Number of filaments	2

Electronic Signature

Purpose

This signature page was created and published because the ACE sign-off action was executed, which is valid for the entire document, including attachments. The ACE sign-off is an electronic signature that requires two distinct identification components: unique username and personal password. The Agilent representative who has delivered this service understands the meaning and legal status of an electronic signature. As a trained official operator, the Agilent representative has a unique password and logon to access ACE and electronically sign this document. (Other e-signatures can be applied to this document using a Document Content Management or other suitable method defined in your data access and control procedures.)

Details

Full Name of Signer:	Supasak Nimsongtham
Logged On User Name:	supasak.nimsongtham@agilent.com
Signature Creation Date:	December 13, 2023
Reason for Signature:	Executed protocol and published this original version of document

Regulatory Disclaimer

This document provides a protocol to verify and record instrument configuration and evidence of proper operation. It has been prepared from our interpretation of applicable regulations as well as industry best practices. The document is designed to provide an important component of a complete compliance package. Validation depends upon many factors and use of this protocol alone does not assure compliance. Agilent Technologies makes no promises or representations as to its sufficiency for any specific regulatory program.

Warranty

Agilent Technologies makes no warranty of any kind to this material, including but not limited to, the implied warranties or merchantability and fitness for a particular purpose. Agilent Technologies shall not be liable for errors contained herein or for incidental or consequential damages in connection with the furnishing, performance, or use of this material.

User Name: supasak.nimsongtham
Report Generated by Hostname: ASBKKWX492

System Id: GM-7
Print Date: December 13, 2023 3:32:47 PM

GM-7-2023 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
December 13, 2023 10:22:24 AM	Audit	SessionCreated	Session	None
December 13, 2023 10:22:24 AM	Start	Configuration	Session	None
December 13, 2023 10:22:24 AM	Audit	Entitlement	Licensing	User is FieldEngineer and does not require an unlock code
December 13, 2023 10:23:53 AM	Audit	Eqpt loaded	Session	EQP details for primary technique [Gc] - File path: [ProtocolPacks/Gc/Configurations/02.50/Gc.02.50.eqp], EQP File Name: [Gc.02.50.eqp], EQP Name: [AgilentRecommended], Protocol Revision : [Gc.02.50] EQP details for hyphenated technique [GcMs] - File path: [ProtocolPacks/GcMs/Configurations/02.50/GcMs.02.50.eqp], EQP File Name: [GcMs.02.50.eqp], EQP Name: [AgilentRecommended]
December 13, 2023 10:23:56 AM	End	Configuration	Session	None
December 13, 2023 10:23:59 AM	Start	Qualification	Session	OQ
December 13, 2023 10:23:59 AM	Start	Execution	System Inspection and Basic Safety and Operation - 7890 - Qualitative Test - No setpoints associated	None

Page 1 / 9

User Name: supasak.nimsongtham

System Id: GM-7

Report Generated by Hostname: ASBKKWX492

Print Date: December 13, 2023 3:32:47 PM

GM-7-2023 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
December 13, 2023 10:24:10 AM	End	Execution	System Inspection and Basic Safety and Operation - 7890: - Qualitative Test - No setpoints associated	Run Count : 1
December 13, 2023 10:24:11 AM	Start	Execution	Inlet Pressure Accuracy - Front SSL: - Pressure Controlled Inlet - S: 25.0 psi - L: <= 1.2 psi	None
December 13, 2023 10:24:15 AM	End	Execution	Inlet Pressure Accuracy - Front SSL: - Pressure Controlled Inlet - S: 25.0 psi - L: <= 1.2 psi	Run Count : 1
December 13, 2023 10:24:17 AM	Start	Execution	GC Oven Temperature Accuracy - 7890: - Temperature - Oven - S: 230.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	None
December 13, 2023 10:32:09 AM	Audit	Data	GC Oven Temperature Accuracy - 7890: - Temperature - Oven - S: 230.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	Manual Data Entry
December 13, 2023 10:32:11 AM	End	Execution	GC Oven Temperature Accuracy - 7890: - Temperature - Oven - S: 230.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	Run Count : 1
December 13, 2023 10:32:12 AM	Start	Execution	GC Oven Temperature Accuracy - 7890: - Temperature - Oven - S: 100.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	None
December 13, 2023 10:34:58 AM	Audit	Data	GC Oven Temperature Accuracy - 7890: - Temperature - Oven - S: 100.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	Manual Data Entry
December 13, 2023 10:34:59 AM	End	Execution	GC Oven Temperature Accuracy - 7890: - Temperature - Oven - S: 100.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	Run Count : 1

Page 2 / 9

User Name: supasak.nimsongtham

System ID: GM-7

Report Generated by Hostname: ASBKKWX492

Print Date: December 13, 2023 3:32:47 PM

GM-7-2023 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
December 13, 2023 10:35:00 AM	Start	Execution	GC Oven Temperature Stability - 7890: - Temperature : Oven - S: 100.0°C - L: <= 0.5°C	None
December 13, 2023 10:35:27 AM	Start	Execution	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 1 - L: >= 1200	None
December 13, 2023 10:36:39 AM	Start	Execution	GC Oven Temperature Stability - 7890: - Temperature : Oven - S: 100.0°C - L: <= 0.5°C	None
December 13, 2023 10:55:10 AM	Audit	Data	GC Oven Temperature Stability - 7890: - Temperature : Oven - S: 100.0°C - L: <= 0.5°C	Manual Data Entry
December 13, 2023 10:55:12 AM	End	Execution	GC Oven Temperature Stability - 7890: - Temperature : Oven - S: 100.0°C - L: <= 0.5°C	Run Count : 1
December 13, 2023 10:55:13 AM	Start	Execution	Log Amp - 5977A SQ: - Source: None EI - Extractor	
December 13, 2023 10:56:42 AM	End	Execution	Log Amp - 5977A SQ: - Source: EI - Extractor	Run Count : 1
December 13, 2023 10:56:43 AM	Start	Execution	RFPA - 5977A SQ: - Source: EI - Extractor	None
December 13, 2023 11:04:44 AM	End	Execution	RFPA - 5977A SQ: - Source: EI - Extractor	Run Count : 1
December 13, 2023 11:04:45 AM	Start	Execution	Tune EI - 5977A SQ: - Source: - None EI - Extractor Filament 1 (Qualitative - No setpoints associated)	
December 13, 2023 11:32:36 AM	End	Execution	Tune EI - 5977A SQ: - Source: - EI - Extractor Filament 1 (Qualitative - No setpoints associated)	Run Count : 1

Page 3 / 9

User Name: supasak.nimsongtham
Report Generated by Hostname: ASBKKWX492

System Id: GM-7
Print Date: December 13, 2023 3:32:47 PM

GM-7-2023 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
December 13, 2023 11:32:38 AM	Start	Execution	Tune EI - 5977A SQ: - Source: - None EI - Extractor Filament 2 (Qualitative - No setpoints associated)	
December 13, 2023 11:33:06 AM	Start	Execution	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 1 - L: >= 1200	None
December 13, 2023 11:49:38 AM	Start	Execution	Tune EI - 5977A SQ: - Source: - None EI - Extractor Filament 2 (Qualitative - No setpoints associated)	
December 13, 2023 11:49:42 AM	End	Execution	Tune EI - 5977A SQ: - Source: - Run Count : 1 EI - Extractor Filament 2 (Qualitative - No setpoints associated)	
December 13, 2023 11:49:43 AM	Start	Execution	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 1 - L: >= 1200	None
December 13, 2023 11:49:48 AM	Audit	AceClosed	Session	None
December 13, 2023 12:36:39 PM	Audit	AceRestarted	Session	None
December 13, 2023 12:36:40 PM	Audit	SessionReloaded	Session	None
December 13, 2023 12:36:42 PM	Start	Qualification	Session	OO
December 13, 2023 12:36:42 PM	Start	Execution	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 1 - L: >= 1200	None

Page 4 / 6

User Name: supasak.nimsongtham
Report Generated by Hostname: ASBKKWX492

System Id: GM-7
Print Date: December 13, 2023 3:32:47 PM

GM-7-2023 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
December 13, 2023 12:37:33 PM	Audit	Data	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 1 - L: >= 1200	Data files Path : D:\MassHunter\GCMS\1\data\1002023\S2N_F1.D
December 13, 2023 12:38:18 PM	End	Execution	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 1 - L: >= 1200	Run Count : 1
December 13, 2023 12:39:51 PM	Audit	TestUnlocked	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 1 - L: >= 1200	Deviation filed for Run Count : 1
December 13, 2023 12:39:51 PM	Start	Execution	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 1 - L: >= 1200	None
December 13, 2023 12:40:15 PM	Audit	Data	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 1 - L: >= 1200	Data files Path : D:\MassHunter\GCMS\1\data\1002023\S2N_F1.D
December 13, 2023 12:42:00 PM	End	Execution	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 1 - L: >= 1200	Run Count : 2
December 13, 2023 12:42:06 PM	Start	Execution	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 2 - L: >= 1200	None
December 13, 2023 12:42:47 PM	Audit	Data	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 2 - L: >= 1200	Data files Path : D:\MassHunter\GCMS\1\data\1002023\S2N_F2.D

User Name: supasak.nimsongtham
Report Generated by Hostname: ASBKKWX492

System Id: GM-7
Print Date: December 13, 2023 3:32:47 PM

GM-7-2023 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
December 13, 2023 12:43:54 PM	End	Execution	Signal to Noise EI - Liquid Injection, Front SSL, SQ - Source: EI - Extractor using Filament 2 - L: >= 1200	Run Count : 1
December 13, 2023 1:54:41 PM	Audit	TestUnlocked	Signal to Noise EI - Liquid Injection, Front SSL, SQ - Source: EI - Extractor using Filament 1 - L: >= 1200	Deviation filed for Run Count : 2
December 13, 2023 1:54:41 PM	Start	Execution	Signal to Noise EI - Liquid Injection, Front SSL, SQ - Source: EI - Extractor using Filament 1 - L: >= 1200	None
December 13, 2023 1:54:50 PM	Audit	Data	Signal to Noise EI - Liquid Injection, Front SSL, SQ - Source: EI - Extractor using Filament 1 - L: >= 1200	Data files Path : D:\MassHunter\GCMS\1\data\10Q2023\52N_F1.D
December 13, 2023 1:55:22 PM	End	Execution	Signal to Noise EI - Liquid Injection, Front SSL, SQ - Source: EI - Extractor using Filament 1 - L: >= 1200	Run Count : 3
December 13, 2023 1:56:50 PM	Audit	TestUnlocked	Signal to Noise EI - Liquid Injection, Front SSL, SQ - Source: EI - Extractor using Filament 1 - L: >= 1200	Deviation filed for Run Count : 3
December 13, 2023 1:56:50 PM	Start	Execution	Signal to Noise EI - Liquid Injection, Front SSL, SQ - Source: EI - Extractor using Filament 1 - L: >= 1200	None
December 13, 2023 2:14:32 PM	Audit	Data	Signal to Noise EI - Liquid Injection, Front SSL, SQ - Source: EI - Extractor using Filament 1 - L: >= 1200	Data files Path : D:\MassHunter\GCMS\1\data\10Q2023\52N_F1.D

Page 6 : 6

User Name: supasak.nimsongtham

System Id: GM-7

Report Generated by Hostname: ASBKKWX492

Print Date: December 13, 2023 3:32:47 PM

GM-7-2023 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
December 13, 2023 2:15:03 PM	End	Execution	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 1 - L: >= 1200	Run Count : 4
December 13, 2023 2:25:07 PM	Audit	TestUnlocked	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 2 - L: >= 1200	Deviation filed for Run Count : 1
December 13, 2023 2:25:07 PM	Start	Execution	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 2 - L: >= 1200	None
December 13, 2023 2:25:20 PM	Audit	Data	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 2 - L: >= 1200	Data files Path : D:\MassHunter\GCMS\1\data\002023\S2N_F2.D
December 13, 2023 2:25:41 PM	End	Execution	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 2 - L: >= 1200	Run Count : 2
December 13, 2023 2:26:51 PM	Audit	TestUnlocked	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 2 - L: >= 1200	Deviation filed for Run Count : 2
December 13, 2023 2:26:51 PM	Start	Execution	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 2 - L: >= 1200	None
December 13, 2023 2:27:01 PM	Audit	Data	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 2 - L: >= 1200	Data files Path : D:\MassHunter\GCMS\1\data\002023\S2N_F2.D

User Name: supasak.nimsongtham
Report Generated by Hostname: ASBKWX492

System Id: GM-7
Print Date: December 13, 2023 3:32:47 PM

GM-7-2023 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
December 13, 2023 2:27:42 PM	End	Execution	Signal to Noise EI - Liquid Injection, Front SSL, SQ - Source: EI - Extractor using Filament 2 - L: >= 1200	Run Count : 3
December 13, 2023 2:29:14 PM	Audit	TestUnlocked	Signal to Noise EI - Liquid Injection, Front SSL, SQ - Source: EI - Extractor using Filament 2 - L: >= 1200	Deviation filed for Run Count : 3
December 13, 2023 2:29:14 PM	Start	Execution	Signal to Noise EI - Liquid Injection, Front SSL, SQ - Source: EI - Extractor using Filament 2 - L: >= 1200	None
December 13, 2023 2:34:02 PM	Start	Execution	Signal to Noise EI - Liquid Injection, Front SSL, SQ - Source: EI - Extractor using Filament 2 - L: >= 1200	None
December 13, 2023 2:41:26 PM	Start	Execution	Signal to Noise EI - Liquid Injection, Front SSL, SQ - Source: EI - Extractor using Filament 2 - L: >= 1200	None
December 13, 2023 2:42:42 PM	Audit	Data	Signal to Noise EI - Liquid Injection, Front SSL, SQ - Source: EI - Extractor using Filament 2 - L: >= 1200	Data files Path : D:\MassHunter\GCMS\1\data\VOQ2023\IS2N_F2_001.D
December 13, 2023 2:44:32 PM	End	Execution	Signal to Noise EI - Liquid Injection, Front SSL, SQ - Source: EI - Extractor using Filament 2 - L: >= 1200	Run Count : 4
December 13, 2023 2:44:56 PM	End	Qualification	Session	OO
December 13, 2023 2:44:56 PM	Start	Reporting	Session	None

User Name: supasak.nimsongtham

System Id: GM-7

Report Generated by Hostname: ASBKKWX492


Print Date: December 13, 2023 3:32:47 PM

GM-7-2023 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
December 13, 2023 3:01:22 PM	Audit	AceClosed	Session	None
December 13, 2023 3:29:10 PM	Audit	AceRestarted	Session	None
December 13, 2023 3:29:10 PM	Audit	SessionReloaded	Session	None
December 13, 2023 3:29:13 PM	Start	Qualification	Session	OQ
December 13, 2023 3:31:33 PM	Audit	Reporting	Session	Report Generated : Certificate
December 13, 2023 3:32:15 PM	Audit	Reporting	Session	Report Generated : Report

Certificate of System Qualification

GC-OQ

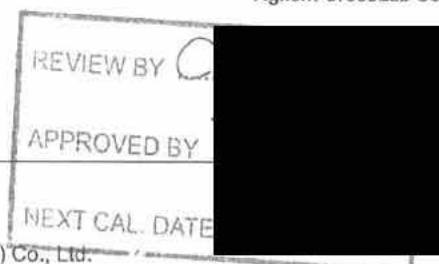

System ID: GC-5
Organization Name: ALS Laboratory Group (Thailand) Co., Ltd.
Organization Location: 104 Phattanakan 40, Phattanakan Rd., Suan Luang, Bangkok 10250

Date: April 21, 2023 9:43:59 AM
EQP Name: AgilentRecommended
EQP Revision: GC.02.52
Overall Qualification Status: Pass

CDS Logon Verification - GC

Logon: Sunee Mongkolvorakijchai

Overall CDS Logon Verification - GC Test Status

Pass

System Inspection and Basic Safety and Operation

Name: 7890
Setpoint Status: Pass

Overall System Inspection and Basic Safety and Operation Test Status

Pass

Inlet Pressure Decay

Name: 7890
Front SSL

Setpoint Status: Pass

Pressure: 25.0 psi

Pressure Change: 0.4 psi /5 minutes

Agilent Recommended: ≥ -2.0 and ≤ 0.5

Date: April 21, 2023 9:43:59 AM
System ID: GC-5

Overall Inlet Pressure Decay Test Status

Pass

Inlet Pressure Accuracy

Name:

7890

Front

SSL

Setpoint Status:

Pass

Setpoint

Actual

Inlet Pressure:

25.0

psi

25.1

psi

Accuracy:

0.1

psi

Agilent Recommended:

<=

1.2

Overall Inlet Pressure Accuracy Test Status

Pass

Detector Flow Accuracy

Name:

7890

Front

FID

Setpoint Status:

Pass

Flow Type:

Fuel

Setpoint:

30.0

mL/min

Measured Flow:

30.5

mL/min

Accuracy:

0.5

mL/min

Agilent Recommended:

<=

10.0

% setpoint

(

3.0

mL/min

)

Limit is percentage of setpoint or 0.5 mL/minute, whichever is largest.

Setpoint Status:

Pass

Flow Type:

Oxidizer

Setpoint:

400.0

mL/min

Measured Flow:

390.6

mL/min

Accuracy:

9.4

mL/min

Agilent Recommended:

<=

10.0

% setpoint

(

40.0

mL/min

)

Limit is percentage of setpoint or 0.5 mL/minute, whichever is largest.

Date:

April 21, 2023 9:43:59 AM

System ID:

GC-5

Setpoint Status:

Flow Type:

Setpoint: mL/min **Measured Flow:** mL/min

Accuracy: mL/min

Agilent Recommended: % setpoint (mL/min)

Limit is percentage of setpoint or 0.5 ml/minute, whichever is largest.

Overall Detector Flow Accuracy Test Status**GC Oven Temperature Accuracy**

Name:

Setpoint Status:

Zone:

Setpoint/Actual

Temperature: °C

Accuracy: °C

Agilent Recommended: % setpoint in K (°C)

% setpoint in K (°C)

Setpoint Status:

Zone:

Setpoint/Actual

Temperature: °C

Accuracy: °C

Agilent Recommended: % setpoint in K (°C)

% setpoint in K (°C)

Overall GC Oven Temperature Accuracy Test Status**GC Oven Temperature Stability**

Name:

Setpoint Status:

Pass

Setpoint/Average

Temperature:

100.0 100.2167 °C

Stability:

0.1 °C

Agilent Recommended:

<= 0.5

Overall GC Oven Temperature Stability Test Status

Pass

Scouting Run

Tested Combination1

Front

SSL

/ Front

FID

Injection Tower

Name:

7683B

Setpoint Status:

Completed

Injection Volume on Column:

1.0 uL

Overall Scouting Run Status

Completed

Noise and Drift

Tested Combination1

Front

SSL

/ Front

FID

Name:

7890

Setpoint Status:

Pass

Base Signal:

18.54 pA

ASTM Noise

pA

0.05

<= 0.10

Drift

pA/Hr

0.10

<= 2.50

Agilent Recommended:

Status:

Pass

Pass

Overall Noise and Drift Test Status

Pass

Date:

April 21, 2023 9:43:59 AM

System ID:

GC-5

Injection Precision

Tested Combination1	Front	SSL	/ Front	FID
Name:	7683B			
Setpoint Status:	Pass			
Injection Volume on Column:	1.0	uL		
Area RSD:	0.56	%	Retention Time RSD:	0.24 %
Agilent Recommended:	<=	3.00	<=	1.00

Overall Injection Precision Test Status

Pass

Signal to Noise

Tested Combination1	Front	SSL	/ Front	FID
	Injection Tower			
Name:	7890			
Setpoint Status:	Pass			
Signal to Noise:	765722			
Agilent Recommended:	>=	300000		

Overall Signal to Noise Test Status

Pass

Instrument Details

Purpose

This section describes the as found system configuration.

Details

System

System ID	GC-5
Manufacturer	Agilent Technologies
Name	7890
Flow Data Input	Manual Data
Temperature Data Input	Manual Data or Other Data Logging

Tested Combination1

Injection Technique	Injection Tower
Inlet	Front
Detector	Front
LTM Included?	No

Sampler 1

Manufacturer	Agilent Technologies
Type	Injection Tower
Name	7683B
Model Number	G2913A
Serial Number	CN00259643
Firmware Revision	A.11.03
Usage	Sample Injection
Location	Front
Syringe Volume (µL)	10

Sampler 2

Manufacturer	Agilent Technologies
Type	Tray
Name	7683A
Model Number	G2614A
Serial Number	CN81347892
Firmware Revision	A.02.01

Mainframe 1

Manufacturer	Agilent Technologies
Name	7890
Model Number	G3440A
Serial Number	US10813027
Firmware Revision	A.01.12.1
Component ID/Asset No.	GC-5
Oven Type	Standard

Inlet 1

Manufacturer	Agilent Technologies
Name	7890
Type	SSL
Location	Front
Carrier Gas	Helium
Control Type	Electronic Pressure Control (EPC)
Purged Inlet	Yes

Detector 1

Manufacturer	Agilent Technologies
Name	7890
Type	FID
Adapter	Capillary
Control Type	Electronic Pressure Control (EPC)
Location	Front
Makeup Gas	Nitrogen

Electronic Signature

Purpose

This signature page was created and published because the ACE sign-off action was executed, which is valid for the entire document, including attachments. The ACE sign-off is an electronic signature that requires two distinct identification components: unique username and personal password. The Agilent representative who has delivered this service understands the meaning and legal status of an electronic signature. As a trained official operator, the Agilent representative has a unique password and logon to access ACE and electronically sign this document. (Other e-signatures can be applied to this document using a Document Content Management or other suitable method defined in your data access and control procedures.)

Details

Full Name of Signer:	Sunee Mongkolvorakijchai
Logged On User Name:	sunee.mongkolvorakijchai@agilent.com
Signature Creation Date:	April 21, 2023
Reason for Signature:	Executed protocol and published this original version of document

Regulatory Disclaimer

This document provides a protocol to verify and record instrument configuration and evidence of proper operation. It has been prepared from our interpretation of applicable regulations as well as industry best practices. The document is designed to provide an important component of a complete compliance package. Validation depends upon many factors and use of this protocol alone does not assure compliance. Agilent Technologies makes no promises or representations as to its sufficiency for any specific regulatory program.

Warranty

Agilent Technologies makes no warranty of any kind to this material, including but not limited to, the implied warranties or merchantability and fitness for a particular purpose. Agilent Technologies shall not be liable for errors contained herein or for incidental or consequential damages in connection with the furnishing, performance, or use of this material.

User Name: sunee.mongkolvorakijchal
 Hostname: 5CG841017D

System Id: GC-5
 Print Date: April 21, 2023 9:44:03 AM

6006075750_OQGC5_ALS Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
April 20, 2023 12:42:57 PM	Audit	SessionCreated	Session	None
April 20, 2023 12:42:57 PM	Start	Configuration	Session	None
April 20, 2023 12:42:57 PM	Audit	Entitlement	Licensing	User is FieldEngineer and does not require an unlock code
April 20, 2023 12:47:02 PM	Audit	EqpLoaded	Session	EQP details for primary technique [Gc] - File path: [ProtocolPacks/Gc/Configurations/02.52/Gc.02.52.eqp], EQP File Name: [Gc.02.52.eqp], EQP Name: [AgilentRecommended], Protocol Revision :[Gc.02.52]
April 20, 2023 12:49:26 PM	End	Configuration	Session	None
April 20, 2023 12:49:31 PM	Start	Qualification	Session	OQ
April 20, 2023 12:49:31 PM	Start	Execution	CDS Logon Verification - GC : - Qualitative test	None
April 20, 2023 3:06:36 PM	Audit	AccClosed	Session	None
April 21, 2023 8:42:16 AM	Audit	AccRestarted	Session	None
April 21, 2023 8:50:30 AM	Audit	SessionReloaded	Session	None
April 21, 2023 8:50:31 AM	Start	Qualification	Session	OQ
April 21, 2023 8:50:31 AM	Start	Execution	CDS Logon Verification - GC : - Qualitative test	None
April 21, 2023 8:51:37 AM	End	Execution	CDS Logon Verification - GC : - Qualitative test	Run Count : 1
April 21, 2023 8:51:39 AM	Start	Execution	System Inspection and Basic Safety and Operation - 7890 : Qualitative Test - No setpoints associated	None

User Name: sunee.mongkolvorakijchal
 Hostname: 5CG841017D

System Id: GC-5
 Print Date: April 21, 2023 9:44:03 AM

6006075750_QQGC5_ALS Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
April 21, 2023 8:52:12 AM	End	Execution	System Inspection and Basic Safety and Operation - 7890: - Qualitative Test - No setpoints associated	Run Count : 1
April 21, 2023 8:52:14 AM	Start	Execution	Inlet Pressure Decay - Front SSL: - Pressure Controlled Inlet - S: 25.0 psi - L: >= -2.0 psi and <= 0.5 psi	None
April 21, 2023 8:53:27 AM	Start	Execution	Inlet Pressure Decay - Front SSL: - Pressure Controlled Inlet - S: 25.0 psi - L: >= -2.0 psi and <= 0.5 psi	None
April 21, 2023 8:53:42 AM	End	Execution	Inlet Pressure Decay - Front SSL: - Pressure Controlled Inlet - S: 25.0 psi - L: >= -2.0 psi and <= 0.5 psi	Run Count : 1
April 21, 2023 8:53:44 AM	Start	Execution	Inlet Pressure Accuracy - Front SSL: - Pressure Controlled Inlet - S: 25.0 psi - L: <= 1.2 psi	None
April 21, 2023 8:53:54 AM	End	Execution	Inlet Pressure Accuracy - Front SSL: - Pressure Controlled Inlet - S: 25.0 psi - L: <= 1.2 psi	Run Count : 1
April 21, 2023 8:53:56 AM	Start	Execution	Detector Flow Accuracy - Front FID: - Type : Fuel - S: 30.0 mL/min - L: <= 10.0% setpoint	None
April 21, 2023 8:54:15 AM	Audit	Data	Detector Flow Accuracy - Front FID: - Type : Fuel - S: 30.0 mL/min - L: <= 10.0% setpoint	Manual Data Entry
April 21, 2023 8:54:19 AM	End	Execution	Detector Flow Accuracy - Front FID: - Type : Fuel - S: 30.0 mL/min - L: <= 10.0% setpoint	Run Count : 1

User Name: sunee.mongkolvorakijchal
 Hostname: 5CG841017D

System Id: GC-5
 Print Date: April 21, 2023 9:44:03 AM

6006075750_OQGC5_ALS Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
April 21, 2023 8:54:22 AM	Start	Execution	Detector Flow Accuracy - Front FID: - Type : Oxidizer - S: 400.0 mL/min - L: <= 10.0% setpoint	None
April 21, 2023 8:54:49 AM	Audit	Data	Detector Flow Accuracy - Front FID: - Type : Oxidizer - S: 400.0 mL/min - L: <= 10.0% setpoint	Manual Data Entry
April 21, 2023 8:54:51 AM	End	Execution	Detector Flow Accuracy - Front FID: - Type : Oxidizer - S: 400.0 mL/min - L: <= 10.0% setpoint	Run Count : 1
April 21, 2023 8:54:54 AM	Start	Execution	Detector Flow Accuracy - Front FID: - Type : Makeup - S: 25.0 mL/min - L: <= 10.0% setpoint	None
April 21, 2023 8:55:21 AM	Audit	Data	Detector Flow Accuracy - Front FID: - Type : Makeup - S: 25.0 mL/min - L: <= 10.0% setpoint	Manual Data Entry
April 21, 2023 8:55:23 AM	End	Execution	Detector Flow Accuracy - Front FID: - Type : Makeup - S: 25.0 mL/min - L: <= 10.0% setpoint	Run Count : 1
April 21, 2023 8:55:25 AM	Start	Execution	GC Oven Temperature Accuracy - 7890: - Temperature : Oven - S: 230.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	None
April 21, 2023 8:57:54 AM	Audit	Data	GC Oven Temperature Accuracy - 7890: - Temperature : Oven - S: 230.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	Manual Data Entry
April 21, 2023 8:57:57 AM	End	Execution	GC Oven Temperature Accuracy - 7890: - Temperature : Oven - S: 230.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	Run Count : 1

User Name: sunee.mongkolvorakijchai
 Hostname: 5CG841017D

System Id: GC-5
 Print Date: April 21, 2023 9:44:03 AM

6006075750_OQGC5_ALS Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
April 21, 2023 8:58:00 AM	Start	Execution	GC Oven Temperature Accuracy - 7890: - Temperature : Oven - S: 100.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	None
April 21, 2023 8:58:41 AM	Audit	Data	GC Oven Temperature Accuracy - 7890: - Temperature : Oven - S: 100.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	Manual Data Entry
April 21, 2023 8:58:43 AM	End	Execution	GC Oven Temperature Accuracy - 7890: - Temperature : Oven - S: 100.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	Run Count : 1
April 21, 2023 8:58:47 AM	Start	Execution	GC Oven Temperature Stability - 7890: - Temperature : Oven - S: 100.0°C - L: <= 0.5°C	None
April 21, 2023 9:00:20 AM	Audit	Data	GC Oven Temperature Stability - 7890: - Temperature : Oven - S: 100.0°C - L: <= 0.5°C	Manual Data Entry
April 21, 2023 9:00:25 AM	End	Execution	GC Oven Temperature Stability - 7890: - Temperature : Oven - S: 100.0°C - L: <= 0.5°C	Run Count : 1
April 21, 2023 9:00:28 AM	Start	Execution	GC Scouting Run - Injection Tower, Front SSL, Front FID: - Part of System Preparation - No limits associated	None
April 21, 2023 9:01:10 AM	Audit	Data	GC Scouting Run - Injection Tower, Front SSL, Front FID: - Part of System Preparation - No limits associated	Data files Path : E:\OQ2023 2023-04-20 15-44-25\SCOUTING.D\FID1 A.ch
April 21, 2023 9:01:51 AM	End	Execution	GC Scouting Run - Injection Tower, Front SSL, Front FID: - Part of System Preparation - No limits associated	Run Count : 1

Page 4 / 6

User Name: sunee.mongkolvorakijchai
 Hostname: 5CG841017D

System Id: GC-5
 Print Date: April 21, 2023 9:44:03 AM

6006075750_OQGC5_ALS Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
April 21, 2023 9:01:55 AM	Start	Execution	Noise and Drift - Front FID: - Detector FID - L (Noise): <= 0.10 pA - L (Drift): <= 2.50 pA/hour	None
April 21, 2023 9:02:21 AM	Audit	Data	Noise and Drift - Front FID: - Detector FID - L (Noise): <= 0.10 pA - L (Drift): <= 2.50 pA/hour	Data files Path : E:\OQ2023 2023-04-20 15-44-25\SIGNSDRF_01.D\FID1A.ch
April 21, 2023 9:02:36 AM	End	Execution	Noise and Drift - Front FID: - Detector FID - L (Noise): <= 0.10 pA - L (Drift): <= 2.50 pA/hour	Run Count : 1
April 21, 2023 9:02:40 AM	Start	Execution	Injection Precision - Injection Tower, Front SSL, Front FID: - GC - L (Area): <= 3.00% - L (Ret. Time): <= 1.00%	None
April 21, 2023 9:03:21 AM	Audit	Data	Injection Precision - Injection Tower, Front SSL, Front FID: - GC - L (Area): <= 3.00% - L (Ret. Time): <= 1.00%	Data files Path : E:\OQ2023 2023-04-20 15-44-25\INJPREC02.D\FID1A.ch
April 21, 2023 9:03:21 AM	Audit	Data	Injection Precision - Injection Tower, Front SSL, Front FID: - GC - L (Area): <= 3.00% - L (Ret. Time): <= 1.00%	Data files Path : E:\OQ2023 2023-04-20 15-44-25\INJPREC03.D\FID1A.ch
April 21, 2023 9:03:21 AM	Audit	Data	Injection Precision - Injection Tower, Front SSL, Front FID: - GC - L (Area): <= 3.00% - L (Ret. Time): <= 1.00%	Data files Path : E:\OQ2023 2023-04-20 15-44-25\INJPREC04.D\FID1A.ch
April 21, 2023 9:03:21 AM	Audit	Data	Injection Precision - Injection Tower, Front SSL, Front FID: - GC - L (Area): <= 3.00% - L (Ret. Time): <= 1.00%	Data files Path : E:\OQ2023 2023-04-20 15-44-25\INJPREC05.D\FID1A.ch

User Name: sunso.mongkolvorakijchai
 Hostname: SCG841017D

System Id: GC-5
 Print Date: April 21, 2023 9:44:03 AM

6006075750_OQGC5_ALS Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
April 21, 2023 9:03:21 AM	Audit	Data	Injection Precision - Injection Tower, Front SSL, Front FID: - GC - L (Area): <= 3.00% - L (Ret. Time): <= 1.00%	Data files Path : E:\OQ2023 2023-04-20 15-44-25\INJPREC06.D\FID1 A.ch
April 21, 2023 9:03:21 AM	Audit	Data	Injection Precision - Injection Tower, Front SSL, Front FID: - GC - L (Area): <= 3.00% - L (Ret. Time): <= 1.00%	Data files Path : E:\OQ2023 2023-04-20 15-44-25\INJPREC07.D\FID1 A.ch
April 21, 2023 9:04:01 AM	End	Execution	Injection Precision - Injection Tower, Front SSL, Front FID: - GC - L (Area): <= 3.00% - L (Ret. Time): <= 1.00%	Run Count : 1
April 21, 2023 9:04:05 AM	Start	Execution	Signal to Noise - Injection Tower, Front SSL, Front FID: - Detector FID - L: >= 300000	None
April 21, 2023 9:04:24 AM	Audit	Data	Signal to Noise - Injection Tower, Front SSL, Front FID: - Detector FID - L: >= 300000	Data files Path : E:\OQ2023 2023-04-20 15-44-25\SIGTON.D\FID1A.ch
April 21, 2023 9:04:38 AM	End	Execution	Signal to Noise - Injection Tower, Front SSL, Front FID: - Detector FID - L: >= 300000	Run Count : 1
April 21, 2023 9:05:27 AM	End	Qualification	Session	OQ
April 21, 2023 9:05:27 AM	Start	Reporting	Session	None
April 21, 2023 9:42:46 AM	Audit	Reporting	Session	Report Generated : Certificate