

ภาคผนวก ฉ

ใบรับรองการสอบเทียบเครื่องมือ



right solutions.
right partner.

รายการเครื่องมือที่ใช้ในการวิเคราะห์ / ทดสอบ

Sample Name	Parameter	Equipment Name	ID No.	Calibrated Date	Next Cal	Freq. Calibrate (Months)
Songkhla Lab	BOD	Incubator	SGK_CL0028	10-Jan-25	10-Jul-26	18
Songkhla Lab	BOD	DO/BOD Analyser	SGK_CL0073	21-May-24	21-Nov-25	18
Songkhla Lab	COD	COD Reactor	SGK_CL0085	15-Jan-25	15-Jan-26	12
Songkhla Lab	COD	Spectrophotometer	SGK_CL0100	25-Dec-24	25-Dec-25	12
Songkhla Lab	pH at 25 °C	pH meter	SGK_CL0030	19-Oct-24	19-Apr-26	18
Songkhla Lab	Oil & Grease	Electronic Top-Loading Balance	SGK_CL0045	10-Jan-25	10-Jan-26	12
Songkhla Lab	Oil & Grease	Oven	SGK_CL0024	19-Oct-24	19-Apr-26	18
Songkhla Lab	Oil & Grease	Water Bath	SGK_CL0035	10-Jan-25	10-Jul-26	18
Songkhla Lab	Total Dissolved Solids 180°C	Electronic Top-Loading Balance	SGK_CL0045	10-Jan-25	10-Jan-26	12
Songkhla Lab	Total Dissolved Solids 180°C	Oven	SGK_CL0024	19-Oct-24	19-Apr-26	18
Songkhla Lab	Total Suspended Solids	Electronic Top-Loading Balance	SGK_CL0045	10-Jan-25	10-Jan-26	12
Songkhla Lab	Total Suspended Solids	Oven	SGK_CL0024	19-Oct-24	19-Apr-26	18
Water Lab	BOD	DO Meter	BKK_EN0017	20-May-25	20-Nov-26	18
Water Lab	BOD	Incubator	BKK_EN0304	4-Mar-25	4-Mar-26	12
Water Lab	BOD	Burette	BKK_EN0422	3-Sep-25	3-Sep-26	12
Water Lab	COD	Hot Block	BKK_EN0222	9-Apr-25	9-Apr-26	12
Water Lab	COD	Spectrophotometer	BKK_EN0356	8-Oct-25	8-Oct-26	12
Water Lab	pH at 25 °C	pH meter	BKK_EN0342	9-Oct-25	9-Oct-26	12
Water Lab	Oil & Grease	Electronic Top-Loading Balance	BKK_EN0003	17-Jul-25	17-Jul-26	12
Water Lab	Oil & Grease	Water Bath	BKK_EN0439	9-Oct-25	9-Oct-26	12
Water Lab	Total Dissolved Solids 180°C	Electronic Top-Loading Balance	BKK_EN0003	17-Jul-25	17-Jul-26	12
Water Lab	Total Dissolved Solids 180°C	Oven	BKK_EN0425	6-Oct-25	6-Oct-26	12
Water Lab	Total Suspended Solids	Electronic Top-Loading Balance	BKK_EN0003	17-Jul-25	17-Jul-26	12
Water Lab	Total Suspended Solids	Oven	BKK_EN0425	6-Oct-25	6-Oct-26	12
Ambient	Total Hydrocarbon	DRYCAL FLOWMETER	BKK_FS0614	9-Sep-24	9-Sep-25	12
Ambient	Total Hydrocarbon	DRYCAL FLOWMETER	BKK_FS0619	9-Sep-24	9-Sep-25	12
Ambient	Total Hydrocarbon	Air Sampling Pump	SGK_FS0153	1-Sep-25	1-Dec-25	3
Ambient	Total Hydrocarbon	Air Sampling Pump	SGK_FS0155	1-Sep-25	1-Dec-25	3
Ambient	Total Hydrocarbon	Air Sampling Pump	SGK_FS0156	1-Sep-25	1-Dec-25	3
Ambient	Total Hydrocarbon	Total Hydrocarbon Analyzer	BKK_FS1068	18-Jun-25	18-Jun-26	12
Ambient	Volatile Organic Compounds	GC-MSD	RYG_EN0136	4-Jul-25	3-Jan-27	18
Ambient	Wind Speed / Wind Direction	Wind Speed / Wind Direction	SGK_FS0088	23-Aug-24	23-Feb-26	18
Ambient	Wind Speed / Wind Direction	Wind Speed / Wind Direction	SGK_FS0035	3-Jul-24	3-Jan-26	18
Ambient	Wind Speed / Wind Direction	Wind Speed / Wind Direction	SGK_FS0036	3-Jul-24	3-Jan-26	18

CALIBRATION CERTIFICATE

Issued Date : 13-Jan-2025

Certificate No. : 25TH0226

CSR No. : A101/05028

Page. : 1 of 3

Customer : ALS Laboratory Group (Thailand) Co., Ltd
114/1 Moo 8, Karnchanawanich Rd. Tambon, Ban Phru,
Amphoe Hat Yai, Songkhla, 90250

Calibration Place : Customer Laboratory

Instrument Name : Incubator

Manufacturer : Memmert

Model : ICP750

Serial No. : F816.0063

ID No. : SGK_CL0028

Resolution : 0.1 °C

Received Date : 10-Jan-2025

Calibrated Date : 10-Jan-2025

Ambient Temperature : (30 ± 10) °C

Relative Humidity : (50 ± 30) %

REVIEW BYAnanta B.....
APPROVED BYKanyda H.....
NEXT CAL. DATE	10/7/26

Calibration Method Used :

This instrument was calibrated using the Calibration In - house method : SCAL.WI.012 based on GLA - 20

The Southern Calibration Service Co.,Ltd.calibration control system complies with requirement of ISO/IEC 17025:2017

Traceability of measurement :

This Certificate is traceable to the International and /or national standards which realize the units of measurement according to the International System of Unit (SI) through :

- TISTR : Thailand Institute of Scientific and Technological Research

Calibrated by : Ibrorhim Saleemin

Approved by :

Imron Rattanaylum / Technical Manager



The uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written approval of Southern Calibration Service Co., Ltd.

Details of Calibration

1. Reference Standard Equipment Used:

Equipment	Model	Serial No.	Cert. no.	Due Date
Data Acquisition/Switch Unit	34970A	MY58009813	PSL-T0707-1/67	22-May-2025


2. The results reported in this certificate refer to the condition of the instrument on the date of calibration and carry no implication regarding the longterm stability of instrument.

3. This certificate is not certified any commercial transaction

4. Condition of Item : normal condition , no indication for any damage or malfunction

Result of Calibration : (✓) Without Adjustment () After Adjustment

1. Sensor Installation Diagram

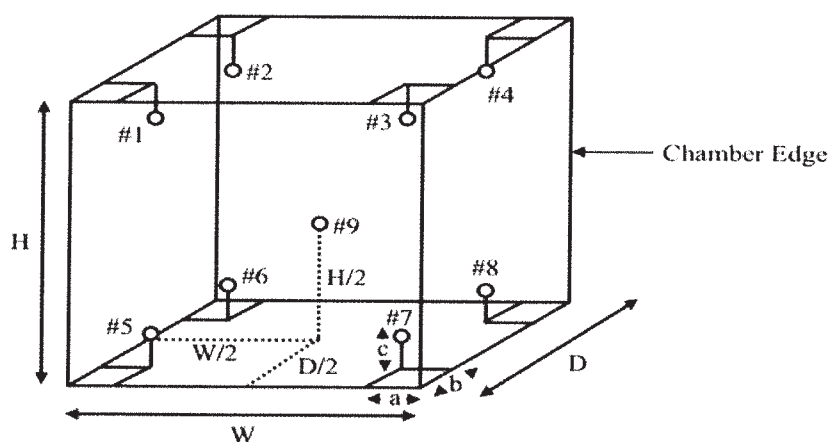

Sensor Installation Details

a = 5.0 cm
b = 5.0 cm
c = 5.0 cm

Dimension of the chamber

W = 104.0 cm
H = 120.0 cm
D = 60.0 cm



Certificate No. : 25TH0226

CSR No. : A101/05028

Page. : 3 of 3

Result of Calibration :

2. Temperature Measurement Accuracy Test

The measurement results of the Incubator and associates are reported in the manner as shown below

Cal point (°C)	Measured Standard Temperature At Spread Locations (°C)									Uncertainty (± °C)
	#1	#2	#3	#4	#5	#6	#7	#8	Ref. 9	
20	20.03	20.23	20.37	20.34	20.32	20.03	20.19	20.31	20.06	0.38

3. Performance Result

The performance of the Incubator are reported as shown below

Cal point (°C)	UUC Setting (°C)	UUC Reading (°C)	Temperature Stability (± °C)	Temperature Uniformity (°C)	Overall Variation (°C)
20	20.0	20.0	0.10	0.31	0.40

- UUC = Unit Under Calibration

The report uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

... End ...



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3 : EQUIPMENT CALIBRATION AND TESTING SERVICES


534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250

TEL. 0-2717-3000 FAX. 0-2719-9484

Certificate of Testing

Cert.No.: 24TW96

Page.: 1 of 2

Equipment :	DO Meter	<div><p>REVIEW BY <u>Ananta B</u></p><p>APPROVED BY <u>Kanitta H</u></p><p>NEXT CAL DATE <u>21/11/25</u></p></div>
Manufacturer :	YSI	
Model :	5000	
Serial No. :	17B101473	
ID No. :	SGK_CL0073	
Received Date :	17 May 2024	
Test Date :	21 May 2024	
Reference :	2405-0608DSC-1	
Submitted by :	ALS Laboratory Group (Thailand) Co.,Ltd. Songkhla Branch. 114/1 Moo 8 Karnchanawanich Rd., T.Ban Phru, A.Hat Yai, Songkhla 90250 Thailand	
Laboratory Condition :	Temperature (25 ± 5) °C Humidity (50 ± 20) %	
Test Procedure :	In - house method : CP-CH9 by Comparison Technique with Azide Modification Method	
Tested by :	Walalak Sirithean	
Approved by :	<div> Approved Signatory</div>	
<div><div><input type="checkbox"/> Unnophol Harachai</div><div><input type="checkbox"/> Ponpan Paipim</div><div><input checked="" type="checkbox"/> Saithip Meangmai</div></div>		
Issue Date :	21 May 2024	



Cert.No.: 24TW96

Page.: 2 of 2

Condition of this result of calibration

1. Reference Standard Instruments :

This certification is traceable to the International System of Unit through the reference standards laboratory of Industrial Calibration Center, Technology Promotion Association (Thailand-Japan).

<u>Instruments</u>	<u>Serial No.</u>	<u>ID No.</u>	<u>Certificate No.</u>	<u>Due Date</u>
1. Burette	-	130BU10	23CG1172	22 Mar 2025
2. Balance	14233821	110RC001	23MM405	16 July 2024

2. Standard Material :-

<u>Material</u>	<u>Manufacturer</u>	<u>Lot.No.</u>	<u>Assay</u>
Sodium Thiosulfate pentahydrate	Merck	AM1763316	100.2%

Result : Dissolved Oxygen Meter Adjustment With Air 100 %

Dissolved Oxygen Probe No.: 17B100103

Titration Method (Azide Modification Method) (mg/L)	DO Meter Reading (mg/L)	Standard Deviation (mg/L)
8.18	8.18	0.0071

This report was certified only for the instrument we tested. It is allowable to use for study. Intend to use for advertising and referral purpose is prohibited. This report may not be reproduced other in full, without written approval of the laboratory.

-o0o-



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL.0-2717-3000-29 FAX.0-2719-9484



Certificate of Calibration

Cert. No.: 24LM77

Page.: 1 of 2

Equipment : DO Meter with Sensor

Manufacturer : YSI

Model : 5000-115

Serial No. : 17B101473

ID No. : SGK_CL0073

Submitted by : ALS Laboratory Group (Thailand) Co.,Ltd.
Songkhla Branch.
114/1 Moo 8 Karnchanawanich Rd.,
T.Ban Phru, A.Hat Yai,
Songkhla 90250 Thailand

Location : TPA On Site Calibration Laboratory

Received Order : 17 May 2024


Calibrated Date : 27 May 2024

Ambient Temperature : (26 ± 10) °C

Relative Humidity : (50 ± 30) %

AC Line Voltage : (220 ± 22) V

Calibrated by : Khit Ruttanaprapachai

Approved by : 
Approved Signatory

() Ponpan Paipim
() Suwit Imjai
(✓) Kunchit Promprat

Issue Date : 28 May 2024

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.



Equipment : DO Meter with Sensor
Condition As-Received : Used Item
Reference : 2405-0608DSC-2
Procedure Used :-

Cert. No.: 24LM77
Page.: 2 of 2

Calibration were conducted using in-house calibration procedure CP-OT01 according to comparison with Industrial Platinum Resistance Thermometer (IPRT) into Temperature Bath.

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

<u>Instrument</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Traceable</u>	<u>Due Date</u>
1) Digital Thermometer	2188080	23I1216	TPA	11 Oct 2024

2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certification is traceable to the International System of Unit.

Remark : TPA : Technology Promotion Association (Thailand - Japan)

Result of Calibration :- (*) Without Adjustment

Function : Temperature measurement.

This instrument was connected with temperature sensor, S/N.: 17B100103

<u>Calibration Point</u> (°C)	<u>Immersion Depth</u> (mm)	<u>Standard Temperature</u> (°C)	<u>UUC* Reading</u> (°C)	<u>Error</u> (°C)	<u>Uncertainty</u> (± °C)	<u>Coverage Factor</u> <i>k</i>
20.00	60	20.005	19.79	-0.215	0.15	2.00

UUC* : Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL.0-2717-3000-29 FAX.0-2719-9484

Certificate of Calibration

Cert. No.: 25TM156

Page.: 1 of 3

Equipment : COD Reactor
Manufacturer : Hach
Model : DRB200
Serial No. : 21120C1313
ID No. : SGK_CL0085

REVIEW BY *Ananta B.*
APPROVED BY *Kanitta H*
NEXT CAL DATE..... 15/01/26

Submitted by : ALS Laboratory Group (Thailand) Co.,Ltd.
(Songkhla Branch)
Karnchanawanich Rd., T.Ban Phru,
A.Hat Yai, Songkhla 90250 Thailand
Location : Chemistry Lab

Received Order : 15 January 2025
Calibration Date : 15 - 16 January 2025
Ambient Temperature : (26 ± 10) °C
Relative Humidity : (50 ± 30) %
AC Line Voltage : (220 ± 22) V

Calibrated by : Uthen Kankawi

Approved by :

S. Suwit
Approved Signatory

() Chakrit Waewwanjua
(✓) Suwit Imjai
() Kunchit Promprat

Issue Date : 06 February 2025

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Calibration and Testing Equipment Services.



Equipment : COD Reactor
Condition As-Received : Used Item
Reference : 2501-0343OC-2
Procedure Used :-

Cert. No.: 25TM156

Page.: 2 of 3

As agreed with customer the calibration was performed using in-house calibration method according to directed measurement method with Data Acquisition which connected with Thermocouple Type T.

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

<u>Instrument</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Traceable</u>	<u>Due Date</u>
1) Data Acquisition	MY44073381	23LM95	TPA	19 Jun 2024

2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certification is traceable to the International System of Unit.


Remark : TPA : Technology Promotion Association (Thailand-Japan), NSC-ONSC Accredited No. Calibration 0008

Result of Calibration :- (*) Without Adjustment

Function of UUC* : Temperature Source

Heat transfer medium used : Alumina Calcined

Environment during calibration		
	Beginning	Finished
Temp.(°C)	22	22
REL.Humi.(%)	56	55
AC Supply (Volt)	225	225

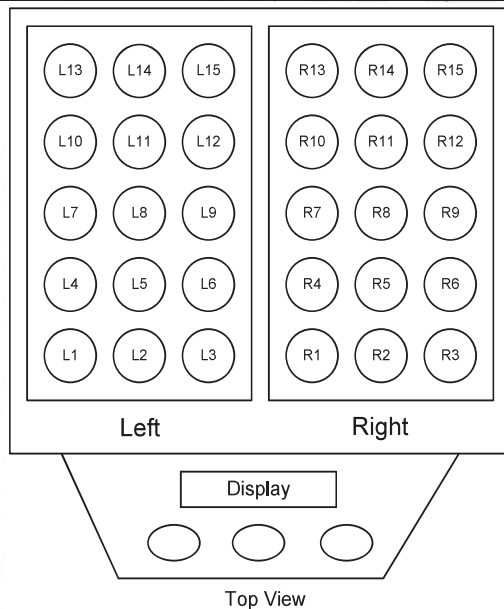

Left		Right	
Position	ID No. of Sensor	Position	ID No. of Sensor
L1	23-01TC-01	R1	23-01TC-01
L2	23-01TC-02	R2	23-01TC-02
L3	23-01TC-03	R3	23-01TC-03
L4	23-01TC-04	R4	23-01TC-04
L5	23-01TC-05	R5	23-01TC-05
L6	23-01TC-06	R6	23-01TC-06
L7	23-01TC-07	R7	23-01TC-07
L8	23-01TC-08	R8	23-01TC-08
L9	23-01TC-09	R9	23-01TC-09
L10	23-01TC-10	R10	23-01TC-10
L11	23-01TC-01	R11	23-01TC-01
L12	23-01TC-02	R12	23-01TC-02
L13	23-01TC-03	R13	23-01TC-03
L14	23-01TC-04	R14	23-01TC-04
L15	23-01TC-05	R15	23-01TC-05



Equipment : COD Reactor
Condition As-Received : Used Item
Reference : 2501-0343OC-2
Result of Calibration :- (*) Without Adjustment
Function of UUC* : Temperature Source
Calibration Point : 150 °C

Cert. No.: 25TM156

Page.: 3 of 3

UUC* Setting (°C)	UUC* Reading (°C)	Measured Temperature (°C)						Temperature stability (± °C)	Uncertainty (± °C)	Coverage Factor <i>k</i>	
		Position									
		Left			Right						
150	150	Left	L13	L14	L15	R13	R14	R15	0.11	1.1	2
			149.407	149.739	149.671	148.510	148.840	148.458			
			L10	L11	L12	R10	R11	R12			
			149.910	150.069	150.171	148.894	148.931	148.753			
			L7	L8	L9	R7	R8	R9			
150	150	Right	150.880	150.841	151.199	150.289	150.358	150.147	0.11		
			L4	L5	L6	R4	R5	R6			
			150.618	150.843	151.109	150.350	150.273	149.820			
			L1	L2	L3	R1	R2	R3			
			150.229	150.688	150.838	150.094	150.115	149.792			

Average* : The average of 30 values in each position.

Temperature stability : One-half of the greatest maximum difference of measured temperature at any one sensor.

UUC* : Unit Under Calibration

Note : The reported uncertainty of measurement was included stability and excluded uniformity .

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

**SCIMET Co., Ltd.**

1194 Soi Wachirathamsathit 57, Bangchak,
Phrakhanong, Bangkok 10260 Thailand
Email:scimet2022@gmail.com, Tel: 02 460 9239
https://www.scimet.co.th



362-cl00100
7/1/25

Certificate No. C07240192

Calibration Certificate

Equipment: SPECTROPHOTOMETER

Model: DR 3900

Serial No.(or ID): 2403637

Manufacturer: HACH

Condition: New

Job No.: KSMT2403543

Received Date: 25 December 2024

Issued Date: 25 December 2024

Page: 1 of 3

Customer

ALS Laboratory Group (Thailand) Co., Ltd
114/1 Moo 8, Karnchanawanich Rd.T. Ban Phru, A Hatyai, Songkhla 90250

Calibration Place

Hach (Thailand) Limited.
Branch 00001, Building D Room No. D3 11, 3rd Floor, No. 735/4, Srinakarin Road,
Pattanakarn, Suanluang, Bangkok 10250 Thailand.

Calibration Date

25 December 2024

Environment Condition

Temperature: 22.2 °C ± 0.5 °C

Humidity: 59.2 %RH ± 2.3 %RH

The Method used

In-house method, WI07, based on ASTM E 275-08 and
ASTM E 387-04

Traceability

This certificate is traceable to the CRM maintained by National Institute
of Standards and Technology (NIST) through Starna Scientific Limited.

The standard for Wavelength Certificate No. 108691 and 108692

The standard for Photometric Certificate No. 109010 , 114655

This certificate is issued the units of
measurement according to the International
System of Units (SI). It provides traceability
of measurement to international or national
standard or other recognized national
standard laboratories.

The measurement uncertainty stated is
the expanded uncertainty which is obtained
from the standard uncertainty multiplied by
the coverage factor ($k=2$) to provide a level
of confidence of approximately 95%. It is
determined in accordance with the Guide to
Expression of Uncertainty in Measurement
(GUM).

These results may be affected by
deviations from specified conditions. The
results relate only to the items tested,
calibrated or sampled. The report shall not
be reproduced except in full without
approval of SCIMET Co., Ltd.


(Mr. Siwaphon Srijan)

Person in charge



(Mr. Thalerngkeat Pongngam)

Authorized signatory


**Condition of reference standards Instruments / CRM:**

<u>Instruments</u>	<u>Set No.</u>	<u>Certificate No.</u>	<u>Due date</u>
Holmium Oxide Glass Reference	121512	108691	25-Jan-25
Didymium Oxide Glass Reference	119722	108692	25-Jan-25
Neutral Density Filter Reference	12276	109010 , 114655	2-Feb-25

Calibration Results:**Without Adjustment**

Wavelength Accuracy (nm), The spectral bandwidth of Std at 5 nm and UUC at 5 nm

Standard Wavelength (nm)	Unit Under Calibration (nm)	Correction (nm)	Uncertainty of Measurement (± nm)
333.67	333	0.67	0.59
361.02	361	0.02	0.59
417.80	417	0.80	0.59
441.29	441	0.29	0.59
479.88	480	-0.12	0.59
513.75	513	0.75	0.59
528.59	528	0.59	0.59
537.75	537	0.75	0.59
585.56	585	0.56	0.59
641.95	642	-0.05	0.59
684.70	685	-0.30	0.59
747.61	748	-0.39	0.59
807.04	807	0.04	0.59
879.68	880	-0.32	0.59

**Calibration Results:****Without Adjustment****Photometric Accuracy (Absorbance)**

Wavelength	Standard absorbance (Abs)	Unit Under Calibration (Abs)	Correction (Abs)	Uncertainty of Measurement(\pm Abs)
420 nm	0.0000	0.000	0.0000	0.0045
	0.2373	0.234	0.0033	0.0045
	0.5617	0.561	0.0007	0.0045
	0.7392	0.738	0.0012	0.0045
	1.0550	1.056	-0.0010	0.0045
440 nm	0.0000	0.000	0.0000	0.0045
	0.2335	0.231	0.0025	0.0045
	0.5513	0.550	0.0013	0.0045
	0.7230	0.722	0.0010	0.0045
	1.0324	1.032	0.0004	0.0045
465 nm	0.0000	0.000	0.0000	0.0045
	0.2126	0.210	0.0026	0.0045
	0.5036	0.506	-0.0024	0.0045
	0.6735	0.676	-0.0025	0.0045
	0.9615	0.965	-0.0035	0.0045
546.1 nm	0.0000	0.000	0.0000	0.0045
	0.2201	0.217	0.0031	0.0045
	0.5176	0.520	-0.0024	0.0045
	0.6930	0.694	-0.0010	0.0045
	0.9908	0.994	-0.0032	0.0045
590 nm	0.0000	0.000	0.0000	0.0045
	0.2443	0.241	0.0033	0.0045
	0.5530	0.554	-0.0010	0.0045
	0.7196	0.719	0.0006	0.0045
	1.0301	1.031	-0.0009	0.0045
635 nm	0.0000	0.000	0.0000	0.0045
	0.2646	0.261	0.0036	0.0045
	0.5370	0.538	-0.0010	0.0045
	0.6862	0.687	-0.0008	0.0045
	0.9822	0.984	-0.0018	0.0045

The End of Certificate

CALIBRATION CERTIFICATE

Issued Date : 22-Oct-2024

Certificate No. : 24CH0526

CSR No. : A163/08133

Page. : 1 of 2

Customer : ALS Laboratory Group (Thailand) Co., Ltd
114/1 Moo 8, Karnchanawanich Rd. Tambon, Ban Phru,
Amphoe Hat Yai, Songkhla, 90250

Calibration Place : Chemical Laboratory

Instrument Name : pH meter

Manufacturer : Mettler Toledo

Model : S220

Serial No. : B625631849

ID No. : SGK_CL0030

Electrode No. : 2281592

Received Date : 19-Oct-2024

Calibrated Date : 19-Oct-2024

Ambient Temperature : $(25 \pm 3) ^\circ\text{C}$

Relative Humidity : $(55 \pm 15) \%$

REVIEW BYAnanta B.....

APPROVED BYKanittha H.....

NEXT CAL. DATE 19/4/26

Calibration Method Used :

This instrument was calibrated using the Calibration In - house method : SCAL.WI.008 based on direct measurement by using certified reference Material (CRM)

The Southern Calibration Service Co.,Ltd.calibration control system complies with requirement of ISO/IEC 17025:2017

Traceability of measurement :

This Certificate is traceable to the International and /or national standards which realize the units of measurement according to the International System of Unit (SI) through :

- CPAchem : CPAchem Ltd
- WK : WK Electric Co., Ltd.
- SCAI : Sounthern Calibration Service Co., Ltd.,

Calibrated by : Alisara Ma

Approved by :

Imron Rattanaylum / Technical Manager



The uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written approval of Southern Calibration Service Co., Ltd.

Details of Calibration
1. Reference Standard Equipment Used:

Equipment	Model	Serial No.	Cert. no.	Due Date
Standard Solution	4.000	61310674	1042701	26-Oct-2025
Standard Solution	7.000	61314184	1042700	26-Oct-2025
Standard Solution	10.01	61313804	1042702	26-Oct-2025
Temperature/Electrical Calibrator	MC2-TE	14987	WK2106-299-223	31-May-2025
Digital Thermometer With Sensor	DP-77	I.360896	24SDTH005	7-Aug-2025

2. The results reported in this certificate refer to the condition of the instrument on the date of calibration and carry no implication regarding the longterm stability of instrument.

3. This certificate is not certified any commercial transaction

4. Condition of Item : normal condition , no indication for any damage or malfunction

Result of Calibration :
1. Electrical Measurement

Applied Voltage (mV)	pH meter Reading		Correction (mV)	Uncertainty (± mV)
	(mV)	(pH)		
177.48	177.5	4.00	-0.02	0.17
0.00	0.0	7.00	0.00	0.13
-177.48	-177.5	10.00	0.02	0.17

2. Before Sample Test Measurement

Standard Buffer Solutions (pH)	pH meter Reading		Correction (pH)	Uncertainty (± pH)
	(pH)	(mV)		
4.007	3.99	178.1	0.017	0.0092
6.976	7.02	1.7	-0.044	0.019
10.009	9.96	-169.6	0.049	0.038

3. After Sample Test Measurement

Standard Buffer Solutions (pH)	pH meter Reading		Correction (pH)	Uncertainty (± pH)
	(pH)	(mV)		
4.007	3.99	177.7	0.017	0.0092
6.976	7.01	3.7	-0.034	0.019
10.009	10.00	-169.0	0.009	0.038

4. Temperature Measurement

Cal Point (°C)	Standard Temperature (°C)	UUC Reading (°C)	Correction (°C)	Uncertainty (± °C)
25	25.021	25.0	0.02	0.060

The report uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

... End ...

CALIBRATION CERTIFICATE

Issued Date : 13-Jan-2025

Certificate No. : 25MA0125

CSR No. : A101/05028

Page. : 1 of 3

Customer : ALS Laboratory Group (Thailand) Co., Ltd
114/1 Moo 8, Karnchanawanich Rd. Tambon, Ban Phru,
Amphoe Hat Yai, Songkhla, 90250

Calibration Place : Customer Laboratory

Instrument Name : Analytical Balance

Manufacturer : Sartorius

Model : MSE224S-100-DU

Serial No. : 34705158

ID No. : SGK_CL0045

Resolution : 0.0001 g

Received Date : 10-Jan-2025

Calibrated Date : 10-Jan-2025

Ambient Temperature : $(30 \pm 10) ^\circ\text{C}$

Relative Humidity : $(50 \pm 20) \%$

REVIEW BY Ananta B
APPROVED BY Kanitha H
NEXT CAL. DATE 10/1/26

Calibration Method Used :

This instrument was calibrated using the Calibration In - house method : SCAL.WI.001 based on UKAS LAB 14 : 2015

The Southern Calibration Service Co.,Ltd.calibration control system complies with requirement of ISO/IEC 17025:2017

Traceability of measurement :

This Certificate is traceable to the International and /or national standards which realize the units of measurement according to the International System of Unit (SI) through :

- SCaL : Sounthern Calibration Service Co., Ltd.,

Calibrated by : Hadbordee Dettawee

Approved by :

Imron Rattanaylum / Technical Manager



The uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written approval of Southern Calibration Service Co., Ltd.

Details of Calibration

1. Reference Standard Equipment Used:

Equipment	Model	Serial No.	Cert. no.	Due Date
Standard Weight Set	2 mg - 1 kg	11119514/01	24SWS001	3-Jul-2025

2. The results reported in this certificate refer to the condition of the instrument on the date of calibration and carry no implication regarding the longterm stability of instrument.

3. This certificate is not certified any commercial transaction

4. Condition of Item : normal condition , no indication for any damage or malfunction

Result of Calibration :. (✓) Without Adjustment () After Adjustment

1. Repeatability

Nominal Value (g)	Standard Deviation (g)
10	0.00000
20	0.00000
200	0.00000

2. Effect of tare

Nominal Value (g)	Standard Value (g)	Balance Reading (g)	Correction (g)
20	20.0000	20.0000	0.0000
40	40.0001	40.0000	0.0001
60	60.0000	60.0000	0.0000
80	80.0001	80.0000	0.0001
100	100.0000	100.0000	0.0000


Result of Calibration :

3. Off-centre loading


A mass approximately 100g was placed on a pan and moved to various position .

The balance reading obtained are given in the table.


Position					Maximum Difference (g)
1	2	3	4	5	
100.0000	100.0000	100.0000	100.0000	100.0001	0.0001



Front



Front



Front

4. Departure from nominal value

Nominal Value (g)	Standard Value (g)	UUC Reading (g)	Correction (g)	Uncertainty (± g)	Coverage Factor (k)
0.01	0.0100	0.0100	0.0000	0.00008	2.0
0.1	0.1000	0.1000	0.0000	0.00008	2.0
0.5	0.5000	0.5000	0.0000	0.00008	2.0
1	1.0000	1.0000	0.0000	0.00008	2.0
2	2.0000	2.0000	0.0000	0.00008	2.0
5	5.0000	5.0000	0.0000	0.00009	2.0
10	10.0000	10.0000	0.0000	0.00009	2.0
20	20.0000	20.0000	0.0000	0.00009	2.0
40	40.0001	40.0000	0.0001	0.00011	2.0
50	50.0000	50.0000	0.0000	0.00013	2.0
60	60.0000	60.0000	0.0000	0.00013	2.0
80	80.0000	80.0000	0.0000	0.00016	2.0
100	100.0000	100.0001	-0.0001	0.00017	2.0
120	120.0000	120.0001	-0.0001	0.00024	2.0
140	140.0001	140.0000	0.0001	0.00024	2.0
160	160.0000	160.0000	0.0000	0.00026	2.0
180	180.0000	180.0000	0.0000	0.00029	2.0
200	200.0000	200.0000	0.0000	0.00030	2.0

- UUC = Unit Under Calibration

The report uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k, providing a level of confidence of approximately 95%

...End...



CALIBRATION CERTIFICATE

Issued Date : 22-Oct-2024

Certificate No. : 24TH4295

CSR No. : A163/08133

Page. : 1 of 3

Customer : ALS Laboratory Group (Thailand) Co., Ltd
114/1 Moo 8, Karnchanawanich Rd. Tambon, Ban Phru,
Amphoe Hat Yai, Songkhla, 90250

Calibration Place : Chemical Laboratory
Instrument Name : Hot Air Oven
Manufacturer : Memmert
Model : UF110
Serial No. : B416.3387
ID No. : SGK_CL0024
Resolution : 0.1 °C
Received Date : 19-Oct-2024
Calibrated Date : 19-Oct-2024
Ambient Temperature : (30 ± 10) °C
Relative Humidity : (50 ± 30) %

REVIEW BYAnanta B.....
APPROVED BYKarnita H.....
NEXT CAL. DATE	19/04/2026

Calibration Method Used :

This instrument was calibrated using the Calibration In - house method : SCAL.WI.012 based on GLA - 20

The Southern Calibration Service Co.,Ltd.calibration control system complies with requirement of ISO/IEC 17025:2017

Traceability of measurement :

This Certificate is traceable to the International and /or national standards which realize the units of measurement according to the International System of Unit (SI) through :

- TISTR : Thailand Institute of Scientific and Technological Research

Calibrated by : Ibrrorhim Saleemin

Approved by :

Imron Rattanaylum / Technical Manager



The uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written approval of Southern Calibration Service Co., Ltd.

Details of Calibration

1. Reference Standard Equipment Used:

Equipment	Model	Serial No.	Cert. no.	Due Date
Data Acquisition/Switch Unit	34970A	MY58009813	PSL-T0707-1/67	22-May-2025

2. The results reported in this certificate refer to the condition of the instrument on the date of calibration

and carry no implication regarding the longterm stability of instrument.

3. This certificate is not certified any commercial transaction


4. Condition of Item : normal condition , no indication for any damage or malfunction

Result of Calibration .:

(✓) Without Adjustment

() After Adjustment

1. Sensor Installation Diagram

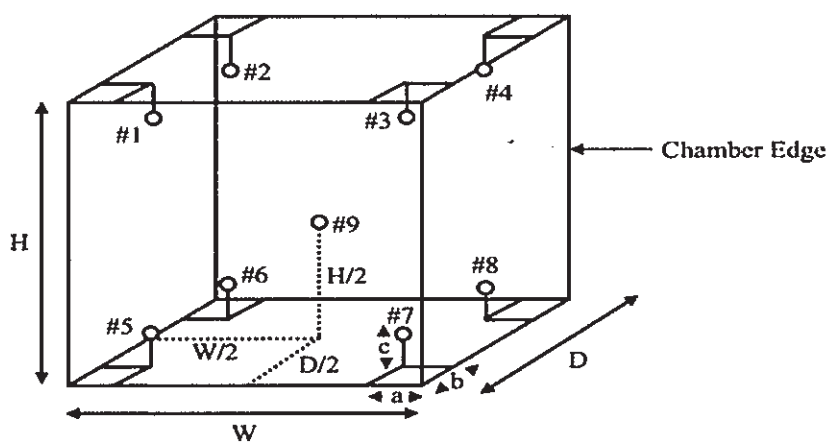

Sensor Installation Details

a = 5.0 cm

b = 5.0 cm

c = 5.0 cm

Dimension of the chamber

W = 55.0 cm

H = 48.0 cm

D = 40.0 cm

Result of Calibration :

2. Temperature Measurement Accuracy Test

The measurement results of the Hot Air Oven and associates are reported in the manner as shown below

Cal point (°C)	Measured Standard Temperature At Spread Locations (°C)									Uncertainty (± °C)
	#1	#2	#3	#4	#5	#6	#7	#8	Ref. 9	
40	40.36	40.40	40.51	40.43	40.05	40.24	40.09	40.14	39.75	0.38
70	70.27	70.30	70.45	70.24	70.24	70.43	70.29	70.30	69.95	0.36
103	102.94	102.90	103.55	102.96	103.22	103.14	103.10	103.01	102.88	0.36
104	104.15	103.99	104.27	104.06	104.09	104.23	104.26	104.15	103.90	0.36
105	105.04	104.90	105.05	104.87	104.91	104.80	104.82	104.98	104.70	0.36
180	179.19	178.93	179.82	179.10	179.27	179.68	179.12	179.73	179.12	0.41

3. Performance Result

The performance of the Hot Air Oven are reported as shown below

Cal point (°C)	UUC Setting (°C)	UUC Reading (°C)	Temperature Stability (± °C)	Temperature Uniformity (°C)	Overall Variation (°C)
40	40.0	40.0	0.20	0.84	0.84
70	70.0	70.0	0.10	0.59	0.59
103	103.0	103.0	0.20	0.73	0.74
104	104.0	104.0	0.20	0.47	0.56
105	105.0	105.0	0.20	0.44	0.46
180	180.0	180.0	0.50	0.86	1.11

- UUC = Unit Under Calibration

The report uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

... End ...

CALIBRATION CERTIFICATE

Issued Date : 13-Jan-2025

Certificate No. : 25TH0227

CSR No. : A101/05028

Page. : 1 of 3

Customer : ALS Laboratory Group (Thailand) Co., Ltd
114/1 Moo 8, Karnchanawanich Rd. Tambon, Ban Phru,
Amphoe Hat Yai, Songkhla, 90250

Calibration Place : Customer Laboratory

Instrument Name : Liquid Bath

Manufacturer : Memmert

Model : WNE29

Serial No. : L616.0538

ID No. : SGK_CL0035

Resolution : 0.1 °C

Received Date : 10-Jan-2025

Calibrated Date : 10-Jan-2025

Ambient Temperature : (30 ± 10) °C

Relative Humidity : (50 ± 30) %

REVIEW BY	Ananta B.
APPROVED BY	Kanitta H.
NEXT CAL. DATE	10/7/26

Calibration Method Used :

This instrument was calibrated using the Calibration In - house method : SCAL.WI.014 based on ASTM E 715 : 1980 (reapproved 2001)

The Southern Calibration Service Co.,Ltd.calibration control system complies with requirement of ISO/IEC 17025:2017

Traceability of measurement :

This Certificate is traceable to the International and /or national standards which realize the units of measurement according to the International System of Unit (SI) through :

- TISTR : Thailand Institute of Scientific and Technological Research

Calibrated by : Ibrorhim Saleemin

Approved by :



Imron Rattanaylum / Technical Manager



The uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written approval of Southern Calibration Service Co., Ltd.

Details of Calibration

1. Reference Standard Equipment Used:

Equipment	Model	Serial No.	Cert. no.	Due Date
Data Acquisition/Switch Unit	34970A	MY58009813	PSL-T0707-1/67	22-May-2025

2. The results reported in this certificate refer to the condition of the instrument on the date of calibration

and carry no implication regarding the longterm stability of instrument.

3. This certificate is not certified any commercial transaction


4. Condition of Item : normal condition , no indication for any damage or malfunction

Result of Calibration .:

(✓) Without Adjustment

() After Adjustment

1. Sensor Installation Diagram

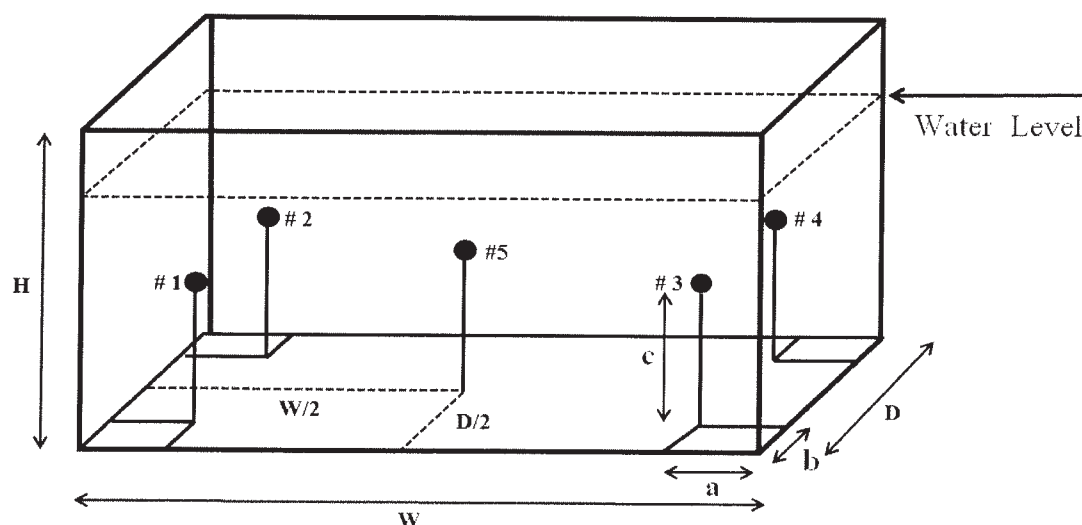

Sensor Installation Details

a = 5 cm
b = 5 cm
c = 5 cm

Dimension of the chamber

W = 59.0 cm
H = 14.0 cm
D = 35.0 cm

Result of Calibration :

2. Temperature Measurement Accuracy Test

The measurement results of the Liquid Bath and associates are reported in the manner as shown below

Cal point (°C)	Measured Standard Temperature At Spread Locations (°C)					Uncertainty (± °C)
	#1	#2	#3	#4	Ref.5	
80	80.05	80.07	79.98	80.05	80.06	0.17

3. Performance Result

The performance of the Liquid Bath are reported as shown below

Cal point (°C)	UUC Setting (°C)	UUC Reading (°C)	Temperature Stability (± °C)	Temperature Uniformity (°C)	Overall Variation (°C)
80	80.0	80.0	0.20	0.17	0.26

- UUC = Unit Under Calibration

The report uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

... End ...



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3 : EQUIPMENT CALIBRATION AND TESTING SERVICES

534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250

TEL. 0-2717-3000 FAX. 0-2719-9484

Certificate of Testing

Cert.No.: 25TW101

Page.: 1 of 2

Equipment :

DO Meter

Manufacturer :

YSI

Model :

5000-230V

Serial No. :

09J101147

ID No. :

BKK_EN0017

Received Date :

19 May 2025

Test Date :

20 May 2025

Reference :

2505-0593DSC-1

Submitted by :

ALS Laboratory Group (Thailand) Co.,Ltd.
104 Phatthanakan 40, Phatthanakan Rd.,
Khwaeng Phatthanakan, Khet Suan Luang,
Bangkok 10250 Thailand

Laboratory Condition :

Temperature (25 ± 5) °C

Humidity (50 ± 20) %

Test Procedure :

In - house method : CP-CH9

by Comparison Technique with Azide Modification Method

Tested by :

Walalak Sirithean

Approved by :

Saithip

Approved Signatory

() Chakrit Waewwanjua

() Ponpan Paipim

(✓) Saithip Meangmai

Issue Date :

20 May 2025

REVIEW BY

finda K

APPROVED BY

Siriluk P

NEXT CAL DATE

20/11/26



Cert.No.: 25TW101

Page.: 2 of 2

Condition of this result of calibration

1. Reference Standard Instruments :

This measurement result is traceable to the International System of Unit through the reference standards laboratory of Industrial Calibration Center, Technology Promotion Association (Thailand-Japan).

<u>Instruments</u>	<u>Serial No.</u>	<u>ID No.</u>	<u>Certificate No.</u>	<u>Due Date</u>
1. Burette	-	130BU10	25CG1126	18 Mar 2027
2. Balance	14233821	110RC001	24MM131	04 July 2025

2. Standard Material :-

<u>Material</u>	<u>Manufacturer</u>	<u>Lot.No.</u>	<u>Assay</u>
Sodium Thiosulfate 5-Hydrate AR	KEMAUS	2203162447	99.6%

Result : Dissolved Oxygen Meter Adjustment With Air 100 %

Dissolved Oxygen Probe No.: 16K100498

Titration Method (Azide Modification Method) (mg/L)	DO Meter Reading (mg/L)	Standard Deviation (mg/L)
8.20	8.21	0.0090

This report was certified only for the instrument we tested. It is allowable to use for study
Intend to use for advertising and referral purpose is prohibited. This report may not be reproduced
other in full, without written approval of the laboratory

-o0o-



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL.0-2717-3000-29 FAX.0-2719-9484



Certificate of Calibration

Cert. No.: 25LM83

Page.: 1 of 2

Equipment : DO Meter with Sensor

Manufacturer : YSI

Model : 5000-230V

Serial No. : 09J101147

ID No. : BKK_EN0017

Submitted by : ALS Laboratory Group (Thailand) Co.,Ltd.
104 Phatthanakan 40, Phatthanakan Rd.,
Khwaeng Phatthanakan, Khet Suan Luang,
Bangkok 10250 Thailand

Location : TPA On Site Calibration Laboratory

Received Order : 19 May 2025

Calibrated Date : 20 May 2025

Ambient Temperature : (26 ± 10) °C

Relative Humidity : (50 ± 30) %

AC Line Voltage : (220 ± 22) V

Calibrated by : Warakorn Lerngagtrakul

Approved by :

Kunchit

Approved Signatory

- () Chakrit Waewwanjua
() Suwit Imjai
(✓) Kunchit Promprat

Issue Date :

26 May 2025

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.



Equipment : DO Meter with Sensor
Condition As-Received : Used Item
Reference : 2505-0593DSC-2

Cert. No.: 25LM83
Page.: 2 of 2

Procedure Used :-

Calibration were conducted using in-house calibration procedure CP-OT01 according to comparison with Industrial Platinum Resistance Thermometer (IPRT) into Temperature Bath.

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

<u>Instrument</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Traceable</u>	<u>Due Date</u>
1) Digital Thermometer	2188080	2411022	TPA	17 Sep 2025

2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certification is traceable to the International System of Unit.

Remark : TPA : Technology Promotion Association (Thailand - Japan)

Result of Calibration :- (*) Without Adjustment

Function : Temperature measurement.

This instrument was connected with temperature sensor, S/N.: 16K100498

<u>Calibration Point</u> (°C)	<u>Immersion Depth</u> (mm)	<u>Standard Temperature</u> (°C)	<u>UUC* Reading</u> (°C)	<u>Error</u> (°C)	<u>Uncertainty</u> (± °C)	<u>Coverage Factor</u> k
20.00	60	20.003	19.92	-0.083	0.15	2.00

UUC* : Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor **k**, providing a level of confidence of approximately 95 %.

-o0o-

Certificate No. T250356


Page 1 of 4

Certificate of Calibration

Equipment : Chamber (Incubator)**Manufacturer** : Memmert**Model** : ICP 750**Serial No.** : F819.0021**Customer Code** : BKK_EN0304**ID No.** : T9572A4**Customer** : ALS Laboratory Group (Thailand) Co.,Ltd.

104 Phatthanakan 40, Phatthanakan Rd.,

Khwaeng Phatthanakan, Khet Suan Luang, Bangkok 10250

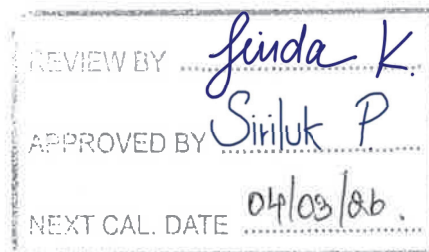Customer Location : Wet Chemistry Lab 2**Date of Receipt** : 26 February 2025**Calibrated By** : Atiphong Rongrat (Technician)**Approved By** :  / Boonchai Suriyawong (Site Calibration Manager)**Date of Issue** : 17 MAR 2025**The uncertainties are for a confidence probability of approximately 95%.**

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standard laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Metrology.

Certificate No. T250356

Page 2 of 4

Calibration Report

Equipment : Chamber (Incubator)
Date of Calibration : 4 March 2025
Environment : Temperature : 24.5-24.7 °C
Line Voltage : 221.4-224.7 V
Relative Humidity : 55 - 65 %RH

Condition of this results of calibration :

1. This equipment was calibrated by insert 12 resistance thermometer detectors into its chamber , the other one resistance thermometer detector use for ambient temperature measurement . The calibration was done in according to WI-T20 (based on ASTM E145-94 (Reapproved 2019) and AS2853-1986).

All data show below were final values and the initial data from customer request . The temperature scale used was based on ITS - 90 .

2. Reference Standard Instrument :

Instrument	Model	Instrument No.	Certificate No.	Due Date
RTD	100 ohm	31-(CH1-10)	T240399	16 March 2025
RTD	100 ohm	32-(CH1-10)	T240399	16 March 2025
DATA LOGGER	34970A	T193	T240399	16 March 2025

3. This certificate is traceable to :

National Institute of Metrology (Thailand) through Metrological Center (NSC-TISI-TIS 17025 CALIBRATION 0244.)

4. Condition of calibrated item : good

Equipment Description :

Time Constant 2 Hour 10 Minute At 20 °C
Fresh Air Damper ☐ Open ☐ Min ☐ Medium ☐ Max
☐ Close
☒ Not Available

5. Adjustment :

(X) without adjustment


() after adjustment

Approved By. 

Certificate No. T250356

Page 3 of 4

Calibration Report

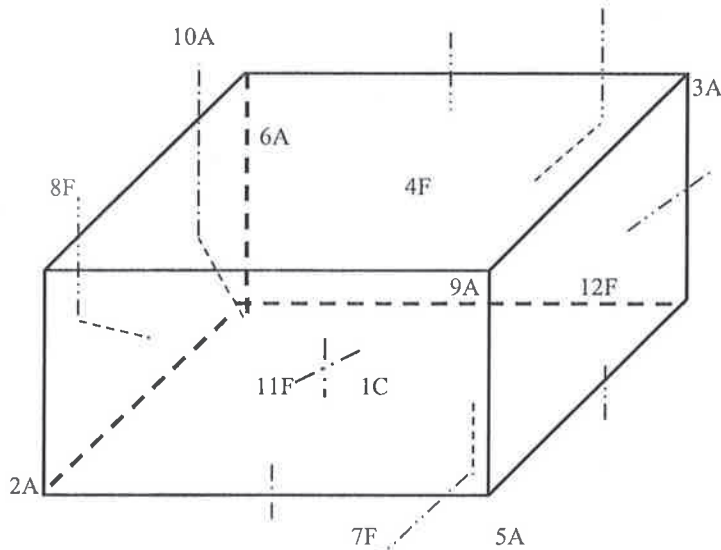

C = Centre , F = Centre of Face , A = Corner , E = Centre of Edge

1C	=	31-CH1
2A	=	31-CH2
3A	=	31-CH3
4F	=	31-CH4
5A	=	31-CH5
6A	=	31-CH6
7F	=	31-CH7
8F	=	31-CH8
9A	=	31-CH9
10A	=	31-CH10
11F	=	32-CH1
12F	=	32-CH2

Approved By. _____



Certificate No. T250356

Page 4 of 4

Calibration Report

Measurement Results :

Calibration Point	Average Standard Reading at each position (°C)											
	31-CH1	31-CH2	31-CH3	31-CH4	31-CH5	31-CH6	31-CH7	31-CH8	31-CH9	31-CH10	32-CH1	32-CH2
20	20.02	20.42	19.96	20.23	19.83	19.44	19.71	20.01	20.06	20.04	20.13	19.98

Chamber (Incubator)			Temperature Distribution				
Setting (°C)	Reading (°C)		Average (°C)	Stability (± °C)	Uniformity (°C)	Uncertainty (± °C)	Coverage Factor <i>k</i>
	Min , Max	Average					
20.0	-	20.0	19.99	0.10	0.43	0.38	2.02

The calibration result apply only the above calibrated item.

The result of test was found accurate as shown on date and place of test only.

The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor *k* which for a t-distribution, providing a level of confidence of approximately 95 % .

End of Certificate

Approved By. 



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL.0-2717-3000-29 FAX.0-2719-9484



Certificate of Calibration

Cert.No.: 25CG3385

Page.: 1 of 2

Equipment :	Burette
Capacity :	50 mL
Serial No. :	-
ID. No. :	BKK_EN0422
Manufacturer :	Witeg
Made in :	Germany
Submitted by :	ALS Laboratory Group (Thailand) Co.,Ltd. 104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan, Khet Suan Luang, Bangkok 10250 Thailand
Ambient Temperature :	(20 ± 2.5) °C
Relative Humidity :	(50 ± 10) %
Barometric Pressure :	753 mmHg
Calibration Procedure :	ASTM E 542 - 01
Calibrated by :	Srisuda Khamtha

REVIEW BY *Liinda K*

APPROVED BY *Siriluk P*

NEXT CAL DATE.....03/09/26

Approved by :

Approved Signatory

() Ponpan Paipim
(✓) Chakrit Waewwanjua

Issue Date :

3 September 2025

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.



Equipment : Burette
Received Date : 1 September 2025
Condition As-Received : Used Item
Calibration Date : 3 September 2025
Reference : 2509-0049DSC-1

Cert.No.: 25CG3385
Page.: 2 of 2

Condition of this result of calibration

1. Reference Standard Instruments :

<u>Instruments</u>	<u>Model</u>	<u>Serial No.</u>	<u>ID. No.</u>	<u>Certificate No.</u>	<u>Traceability</u>	<u>Due date</u>
1) Balance	MS204TS	C226356983	140RC010	24MM603	TPA	10 Oct 2025
2) Data Logger	HL-20D	20683159	140EC012	24H2129	TPA	15 Oct 2025
3) Digital Thermometer	HH376	230806555	140EC013	25I1740	TPA	17 Jan 2026

This measurement result is traceable to SI Unit

2. The certificate is valid only to the item calibrated on date and place of calibration.
3. True value is converted to true volume at the standard temperature of 20 °C

Calibration result :

Nominal capacity (mL)	Reading (mL)	Uncertainty (± mL)	k Factor
10	9.9941	0.0082	2.00
25	24.9804	0.0087	2.00
50	49.9819	0.010	2.00

Remark mL = cm³

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k , providing a level of confidence of approximately 95 %.

-o0o-

Certificate No. T250579

Page 1 of 5

Certificate of Calibration

Equipment : HOT BLOCK

Manufacturer : Environmental Express

Model : B3000- 240

Serial No. : 2017CODW116

Customer Code : BKK_EN0222

ID No. : T6769A4

Customer : ALS Laboratory Group (Thailand) Co.,Ltd.

104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan,
Khet Suan Luang, Bangkok 10250

Customer Location : Wet Chemistry Lab2

Date of Receipt : 2 April 2025

Calibrated By : Boonchai Suriyawong (Site Calibration Manager)

Approved By :  / Sujjar Naknakred (Site Calibration Manager)

Date of Issue : 21 APR 2025

REVIEW BY	<i>Jinda K</i>
APPROVED BY	<i>Siriluk P</i>
NEXT CAL. DATE	09/04/26

The uncertainties are for a confidence probability of approximately 95%.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standard laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Metrological Center.

Certificate No. T250579

Page 2 of 5

Calibration Report

Equipment : HOT BLOCK
Date of Calibration : 9 April 2025
Environment : Temperature : 22.8-22.9 °C
 Line Voltage : 222.1-225.1 V
 Relative Humidity : 55 - 65 %RH

Condition of this results of calibration :

1. This equipment was calibrated by insert 20 standard thermocouples type T into its chamber , the other one standard thermocouples type T use for ambient temperature measurement . The calibration was done in according to WI-T20

All data show below were final values and the initial data from customer request . The temperature scale used was based on ITS - 90 .

2. Reference Standard Instrument :

Instrument	Model	Instrument No.	Certificate No.	Due Date
TC	TYPE T	TN91-TN100	T242036	3 December 2025
TC	TYPE T	TN101-TN110	T242036	3 December 2025
DATA LOGGER	34970A	T121	T242036	3 December 2025

3. This certificate is traceable to :

National Institute of Metrology (Thailand) through Metrological Center (NSC-TISI-TIS 17025 CALIBRATION 0244.)

4. Condition of calibrated item : good

Equipment Description :

Time Constant - Hour 40 Minute At 150 °C
 Fresh Air Damper ☐ Open ☐ Min ☐ Medium ☐ Max
☐ Close
☒ Not Available

5. Adjustment :

(X) without adjustment

() after adjustment


Approved By.



Certificate No T250579

Page 3 of 5

Calibration Report

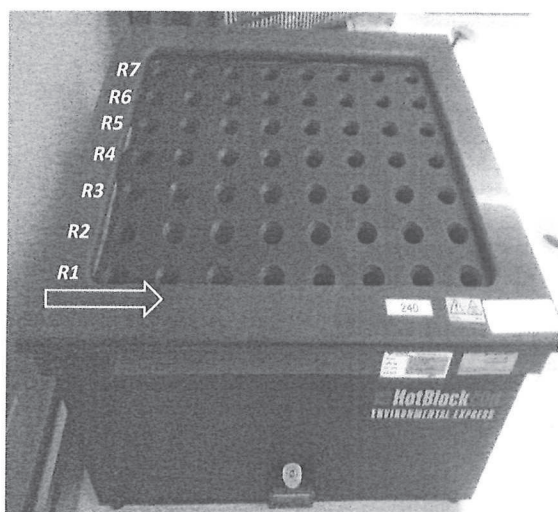

Row	Hole							
R7	H49	H50	H51	H52	H53	H54	H55	H56
R6	H41	H42	H43	H44	H45	H46	H47	H48
R5	H33	H34	H35	H36	H37	H38	H39	H40
R4	H25	H26	H27	H28	H29	H30	H31	H32
R3	H17	H18	H19	H20	H21	H22	H23	H24
R2	H9	H10	H11	H12	H13	H14	H15	H16
R1	H1	H2	H3	H4	H5	H6	H7	H8

H: STANDARD THERMOCOUPLE TYPE T

H1	=	TN91	H9	=	TN99	H17	=	TN107	H25	=	TN95	H33	=	TN103	H41	=	TN91	H49	=	TN99
H2	=	TN92	H10	=	TN100	H18	=	TN108	H26	=	TN96	H34	=	TN104	H42	=	TN92	H50	=	TN100
H3	=	TN93	H11	=	TN101	H19	=	TN109	H27	=	TN97	H35	=	TN105	H43	=	TN93	H51	=	TN101
H4	=	TN94	H12	=	TN102	H20	=	TN110	H28	=	TN98	H36	=	TN106	H44	=	TN94	H52	=	TN102
H5	=	TN95	H13	=	TN103	H21	=	TN91	H29	=	TN99	H37	=	TN107	H45	=	TN95	H53	=	TN103
H6	=	TN96	H14	=	TN104	H22	=	TN92	H30	=	TN100	H38	=	TN108	H46	=	TN96	H54	=	TN104
H7	=	TN97	H15	=	TN105	H23	=	TN93	H31	=	TN101	H39	=	TN109	H47	=	TN97	H55	=	TN105
H8	=	TN98	H16	=	TN106	H24	=	TN94	H32	=	TN102	H40	=	TN110	H48	=	TN98	H56	=	TN106

Approved By.



Certificate No. T250579

Page 4 of 5

Calibration Report

Measurement Results

			Average Standard Reading at each position (°C)									
Calibration Point			TN91	TN92	TN93	TN94	TN95	TN96	TN97	TN98	TN99	TN100
150	150.2	Max	150.48	150.03	149.42	150.76	149.50	150.44	149.78	149.96	150.02	150.35
		Min	150.30	149.86	149.23	150.57	149.29	150.24	149.62	149.75	150.20	150.20
		Average	<i>150.40</i>	<i>149.94</i>	<i>149.34</i>	<i>150.67</i>	<i>149.40</i>	<i>150.34</i>	<i>149.71</i>	<i>149.86</i>	<i>149.95</i>	<i>150.29</i>
			TN101	TN102	TN103	TN104	TN105	TN106	TN107	TN108	TN109	TN110
		Max	150.08	150.18	150.18	150.56	150.01	149.33	149.76	150.52	150.65	150.02
		Min	149.94	150.03	150.16	150.37	149.80	149.09	149.64	150.40	150.50	149.83
		Average	<i>150.03</i>	<i>150.11</i>	<i>150.25</i>	<i>150.48</i>	<i>149.91</i>	<i>149.20</i>	<i>149.70</i>	<i>150.46</i>	<i>150.58</i>	<i>149.92</i>
			TN91	TN92	TN93	TN94	TN95	TN106	TN97	TN98	TN99	TN100
		Max	149.41	149.87	149.17	149.78	149.61	150.30	149.32	150.32	150.02	150.22
		Min	149.31	149.74	149.00	149.63	149.50	150.18	149.18	150.23	149.89	150.12
		Average	<i>149.35</i>	<i>149.79</i>	<i>149.10</i>	<i>149.72</i>	<i>149.56</i>	<i>150.23</i>	<i>149.27</i>	<i>150.28</i>	<i>149.97</i>	<i>150.17</i>
			TN101	TN102	TN103	TN104	TN105	TN106	TN107	TN108	TN109	TN110
		Max	149.63	149.57	150.11	149.69	149.91	149.55	149.59	150.27	150.06	149.53
		Min	149.52	149.45	149.98	149.60	149.76	149.41	149.44	150.18	149.95	149.42
		Average	<i>149.58</i>	<i>149.51</i>	<i>150.06</i>	<i>149.64</i>	<i>149.85</i>	<i>149.49</i>	<i>149.53</i>	<i>150.22</i>	<i>150.00</i>	<i>149.49</i>
			TN91	TN92	TN93	TN94	TN95	TN96	TN97	TN98	TN99	TN100
		Max	149.36	149.62	149.48	150.45	149.58	150.12	149.10	149.91	149.66	150.15
		Min	149.18	149.45	149.34	150.33	149.52	150.06	149.01	149.87	149.49	150.04
		Average	<i>149.29</i>	<i>149.54</i>	<i>149.41</i>	<i>150.39</i>	<i>149.56</i>	<i>150.09</i>	<i>149.06</i>	<i>149.89</i>	<i>149.60</i>	<i>150.11</i>
			TN101	TN102	TN103	TN104	TN105	TN106				
		Max	149.71	149.73	150.63	148.58	149.83	149.13				
		Min	149.59	149.66	150.53	148.46	149.79	149.07				
		Average	<i>149.65</i>	<i>149.70</i>	<i>150.59</i>	<i>149.75</i>	<i>149.17</i>	<i>149.10</i>				

Approved By.



Certificate No. T250579

Page 5 of 5

Calibration Report

Measurement Results

HOT BLOCK			Temperature Distribution	
Setting (°C)	Reading (°C)		Stability (\pm °C)	Uncertainty (\pm °C)
	Min , Max	Average		
150.2	150.2 , 150.3	150.2	0.20	0.82

The calibration result apply only the above calibrated item.

The result of test was found accurate as shown on date and place of test only.

The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor $k=2$, providing a level of confidence of approximately 95 % .

End of Certificate

 Approved By. 



Certificate of Calibration

Cert.No.: 25CHO537

Page.: 1 of 3

Equipment : Spectrophotometer
Manufacturer : HACH
Model : DR3900
Serial No. : 2021559
ID No. : BKK_EN0356
Condition As-Received: Used Item
Received Date : 08 October 2025
Calibration Date : 08 October 2025
Reference : 2510-0042OC-11
Submitted by : ALS Laboratory Group (Thailand) Co.,Ltd.
104 Phatthanakan 40, Phatthanakan Rd.,
Khwaeng Phatthanakan, Khet Suan Luang,
Bangkok 10250 Thailand
Calibration Place : Wet Chemistry Lab 2
Ambient Temperature : (21.9 to 21.9) °C (On-Site)
Relative Humidity : (62 to 65) % (On-Site)
Calibration Procedure : In - house method :
CP-OCH4 based on ASTM E 275-08
Calibrated by : Uthen Kankawi
Approved by : 
() Chakrit Waewwanjua
() Ponpan Paipim
(✓) Saithip Meangmai
Issue Date : 9 October 2025

REVIEW BY 

APPROVED BY 

NEXT CAL DATE... 08/10/26

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.



Cert. No. : 25CHO537

Page : 2 of 3

Condition of calibration result

1. Reference Standard Material :

<u>Material</u>	<u>Serial No.</u>	<u>Certificate No.</u>	<u>Due date</u>
1. Absorbance Standard set	44487	122584	31 May 2026
2. Wavelength Standard set	36730	118120	15 Jan 2026
3. Wavelength Standard set	36730	118121	15 Jan 2026

2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certificate is traceable to the International System of Unit maintained through :

- Starna Scientific Ltd.

4. Spectral BandWidth : 5 nm
Scan Speed : - nm/min

Calibration Results : without adjustment

Wavelength Accuracy

Certified Values of Reference Material (nm)	UUC Reading (nm)	Uncertainty of Measurement (\pm nm)	Coverage Factor <i>k</i>
418.40	418	0.59	2.00
479.88	480	0.59	2.00
513.75	513	0.59	2.00
537.00	536	0.59	2.00
638.00	638	0.59	2.00
747.61	748	0.59	2.00
807.04	807	0.59	2.00



Cert. No. : 25CHO537

Page : 3 of 3

Calibration Results : without adjustment

Photometric Accuracy

Wavelength (nm)	Certified Values of Reference Material (Abs)	UUC Reading (Abs)	Uncertainty of Measurement (\pm Abs)	Coverage Factor <i>k</i>
420.0	Zero	0.000	0.0028	2.00
	0.5750	0.573	0.0028	2.00
	0.7156	0.713	0.0028	2.00
	1.0176	1.014	0.0028	2.00
440.0	Zero	0.000	0.0028	2.00
	0.5598	0.557	0.0028	2.00
	0.7037	0.700	0.0028	2.00
	1.0013	0.997	0.0028	2.00
465.0	Zero	0.000	0.0028	2.00
	0.5222	0.522	0.0028	2.00
	0.6646	0.664	0.0028	2.00
	0.9444	0.945	0.0028	2.00
546.1	Zero	0.000	0.0028	2.00
	0.5234	0.523	0.0028	2.00
	0.7007	0.700	0.0028	2.00
	0.9992	0.999	0.0028	2.00
590.0	Zero	0.000	0.0028	2.00
	0.5573	0.556	0.0028	2.00
	0.7760	0.773	0.0028	2.00
	1.1104	1.108	0.0028	2.00
635.0	Zero	0.000	0.0028	2.00
	0.5648	0.565	0.0028	2.00
	0.7654	0.765	0.0028	2.00
	1.0961	1.096	0.0028	2.00

Remark

- Each individual filter is measured against the empty filter holder (blank) used to zero the spectrophotometer
- UUC = Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k* , providing a level of confidence of approximately 95 %.



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL.0-2717-3000-29 FAX.0-2719-9484



Certificate of Calibration

Cert.No.: 25CH1162

Page.: 1 of 3

Equipment : pH Meter
Manufacturer : Hach
Model : HQ411d
Serial No. : 200100031163
ID No. : BKK_EN0342
Condition As-Received: Used Item
Received Date : 08 October 2025
Calibration Date : 09 October 2025
Reference : 2510-0271DSC-1
Submitted by :

Ambient Temperature : $(25 \pm 2.5) ^\circ\text{C}$
Relative Humidity : $(50 \pm 15) \%$
Calibration Procedure :
In - house method :
- CP-CH5 by direct measurement with
certified reference material (CRM)
- CP-CH8 by comparison with temperature standard

Calibrated by : Walalak Sirithean

Approved by :

Saithip

Approved Signatory

- () Chakrit Waewwanjua
() Ponpan Paipim
(✓) Saithip Meangmai

Issue Date : 10 October 2025

REVIEW BY *Jinda K*
APPROVED BY *Siriluk P*
NEXT CAL DATE..... 09/10/26

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.



Cert.No.: 25CH1162

Page.: 2 of 3

Condition of this calibration result

1. Reference Standard Instrument

<u>Instrument</u>	<u>Serial No.</u>	<u>ID No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
1) Ref. Standard Thermometer	4982054	110RC044	25I708	03 July 2026

- This measurement result is traceable to SI through Technology Promotion Association (Thailand - Japan)

2. Certified Reference Materials : The measurement results are traceable to SI through CPA chem Ltd.,
ANSI-ASQ National Accreditation Board, Accredited No. AR-1835

<u>Buffer Solution</u>	<u>Manufacturer</u>	<u>Lot No.</u>	<u>Exp. date</u>
pH 4.007	CPA chem	1114384	12 June 2027
pH 6.965	CPA chem	1066667	18 Jan 2026
pH 10.010	CPA chem	1135355	16 Aug 2026

3. This certificate is valid only to the item calibrated on date and place of calibration.

Calibration Results

Function : pH Measurement

Performing three buffers standard curve by using buffer nominal pH (4,7,10)

Unit Under Calibration	Standard pH Buffer Solution	Actual pH Reading	Actual mV Reading (mV)	Uncertainty of pH Measurement (\pm)	Coverage factor k
pH Electrode S/N.: 252063043080	4.007	3.996	176.6	0.0046	2.00
	6.965	6.974	1.1	0.0084	2.00
	10.010	9.996	-176.9	0.0070	2.00

Remark - Can not connect the BNC because the plug does not match with the socket.



Cert.No.: 25CH1162

Page.: 3 of 3

Calibration Results

Function : Temperature Measurement

(*) Without adjustment

This equipment was connected with Temperature Probe;

- Model : PHC281

- Serial No. : 252063043080

Dimension of probe

- Length : 103 mm.

- Diameter : 12 mm.

- Immersion Depth : 90 mm.

Calibration Point (°C)	Standard Temperature (°C)	UUC* Reading (°C)	Error (°C)	Uncertainty of measurement (± °C)	Coverage factor <i>k</i>
25.0	25.001	25.0	-0.001	0.13	2.00

Remark - UUC* = Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

Accredited by

NSC-TISI-TIS 17025

Calibration 0426



NSC-TISI-TIS 17025

CALIBRATION 0426

Calibration certificate

Calibration Certificate No. 25BCI0265

Object	Electronic non-automatic weighing instrument	This calibration certificate documents the traceability to national standards.
Manufacturer	Sartorius	Uncertainties of measurements are taken into account when only statements of compliance are made.
Type	MSE224S-100-DU	This certificate was prepared by Sartorius Corporation in accordance to the current ISO/IEC 17025:2017 standard and Sartorius Work Instruction (Method) SOP WI 08.
Serial QM Ident. no.	27405555 BKK_EN0003	This certificate relate and apply this equipment only.
Customer	ALS Laboratory Group (Thailand)Co., Ltd. 104 Phatthanakarn 40,Phattanakarn Rd.,Khwaeng Phatthanakarn ,Khet Suan Luang,Bangkok 10250	<div>REVIEW BY <i>Linda K</i></div> <div>APPROVED BY <i>Siriluk P</i></div> <div>NEXT CAL DATE.....17/07/26</div>
Order no.	265054	
Number of pages	4	
Date of calibration	17 Jul 2025	

This calibration certificate may not be reproduced other than in full except with the permission of NSC-TISI-TIS-17025 and the issuing laboratory. Calibration certificates without signature are not valid.

The user is obliged to have the object recalibrated at appropriate intervals.

Date of issue	17 Jul 2025	Approval of the Calibration Certificate	Person in charge
		Mr. Chonchai Inthana	Chonchai Inthana

Calibration object

Single range instrument

Model	MSE224S-100-DU
Serial Number	27405555
QM Ident. no Inventory no.	BKK_EN0003 ---

Maximum capacity (Max. load)	220.0000 g
Measured up to	220.0000 g
Scale interval	0.0001 g

Place of calibration

Address	According to page 1
Department Cost center	ENVI Department ---
Building Floor	--- 1st Floor.
Room	Laboratory Room.
Maximum temperature variation at place of calibration	5 K

Calibration procedure

EURAMET Calibration Guide No. 18, Version 4.0 (11/2015) - Guidelines on the Calibration of Non-Automatic Weighing Instruments

Test equipment

Test equipment type	Test equipment ID	Valid until
Thermometer	Testo 174(Traceable to Si unit through ENTECH)	11 Nov 2025
Test weight set OIML R111 E2	Certificate No.M2308197S ,E2(Traceable to SI unit through TCS)	23 Aug 2025

Adjustment Status

The measuring device was internally adjusted before the calibration.

Environmental and measuring conditions

Date of calibration	17 Jul 2025
Temperature at place of calibration Temp. diff. <i>T</i> _{weights} - <i>T</i> _{place}	22.5 °C 0.7 K
Measuring conditions	The installation site is suitable. The device is level. Balance was loaded up to Max before test.
Comments	Humidity 58.0 %RH.

Measurement results | Measurement uncertainties

Repeatability

Test load (nominal): 10 g 200 g		
	10 g	200 g
1	10.0000 g	200.0000 g
2	10.0000 g	199.9999 g
3	10.0000 g	200.0000 g
4	10.0000 g	200.0000 g
5	10.0001 g	199.9999 g
6	10.0000 g	200.0000 g
7	10.0000 g	200.0000 g
8	10.0001 g	200.0000 g
9	10.0000 g	200.0000 g
10	10.0000 g	199.9999 g
	<i>s</i> = 0.00004 g	<i>s</i> = 0.00005 g

Eccentricity

Test load (nominal): 100 g	
Center	100.0000 g
Front left	100.0001 g
Back left	100.0000 g
Back right	100.0001 g
Front right	100.0001 g
Maximum deviation from centric loading indication $ \Delta_{ecc} _{max} = 0.0001\text{ g}$	

Error of indication

Testload	Indication	Error	Expansion factor	Uncertainty	Uncertainty relative
<i>L</i>	<i>I</i>	<i>E</i>	<i>k</i>	<i>U</i> (<i>E</i>)	<i>U</i> _{rel} (<i>E</i>)
0.0100 g	0.0100 g	0.0000 g	2.00	0.00012 g	1.2 %
0.1000 g	0.1000 g	0.0000 g	2.00	0.00013 g	0.13 %
1.0000 g	1.0000 g	0.0000 g	2.00	0.00013 g	0.013 %
2.0000 g	2.0000 g	0.0000 g	2.00	0.00013 g	0.0065 %
5.0000 g	5.0000 g	0.0000 g	2.00	0.00013 g	0.0026 %
10.0000 g	10.0000 g	0.0000 g	2.00	0.00013 g	0.0013 %
20.0000 g	20.0000 g	0.0000 g	2.00	0.00014 g	0.00068 %
50.0000 g	50.0000 g	0.0000 g	2.00	0.00015 g	0.00029 %
100.0000 g	100.0000 g	0.0000 g	2.00	0.00018 g	0.00018 %
200.0000 g	200.0000 g	0.0000 g	2.00	0.00028 g	0.00014 %
220.0000 g	220.0001 g	0.0001 g	2.00	0.00032 g	0.00015 %
Maximum error of indication		$ E _{max} = 0.0001\text{ g}$			

*U*_{rel}(*E*) is the quotient of *U*(*E*) and test load *L*. The uncertainty of measurement *U*(*E*) is valid only if error *E* is considered. You will find reference notes on the uncertainty of measurement in use under: Appendix to the calibration certificate | Interpretation of measurement results.
Reference note: The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the documented Expansion factor, determined in accordance with the European Calibration Guideline EURAMET cg-18, V4.0. There is a 95 % probability that the value of the measurand will be in the assigned value range.

End of calibration certificate

Uncertainty of measurement in use

Device adjusted before measurement	Yes
Temperature deviation considered	1.5 K (isoCAL active)
Temperature coefficient considered	$1 \cdot 10^{-6}/\text{K}$


Uncertainty of the weighing result $U_{gl}(W)$

$U_{gl}(W) = 0.00013 \text{ g} + 4.19 \cdot 10^{-6} \cdot R$

Reference note: The current uncertainty of measurement is calculated by entering of the reading R into this formula. In relation to this, there is no need for a correction of the indication error. The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied with an Expansion factor of 2, determined in accordance with the European Calibration Guideline EURAMET cg-18, V4.0. There is a 95 % probability that the value of the measurand will be in the assigned value range.

Indication in % from max load	Net indication R	Uncertainty $U_{gl}(W)$	Uncertainty relative $U_{gl}(W)_{rel}$
1 %	2.2000 g	0.00014 g	0.0063 %
25 %	55.0000 g	0.00036 g	0.00066 %
50 %	110.0000 g	0.00059 g	0.00054 %
75 %	165.0000 g	0.00082 g	0.00050 %
100 %	220.0000 g	0.0011 g	0.00048 %

Graphic realization of the relative uncertainty of measurement | process accuracy

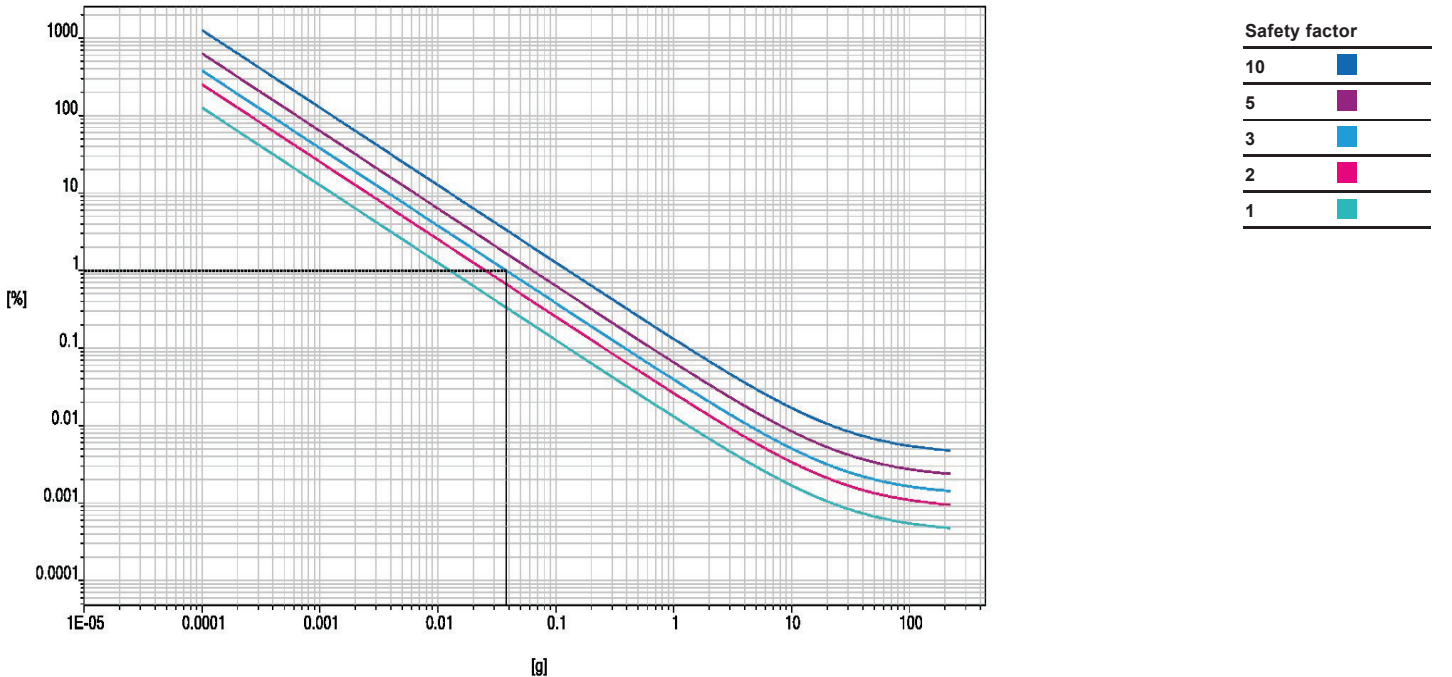

Displayed example

Process accuracy	1.00 %
Safety factor	3
Minimum sample weight	0.0380 g



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL.0-2717-3000-29 FAX.0-2719-9484



Certificate of Calibration

Cert. No.: 25TM528

Page : 1 of 3

Equipment : Water Bath
Manufacturer : Memmert
Model : WNE 29
Serial No. : L622.0282
ID No. : BKK_EN0439

REVIEW BY

Jinda K

APPROVED BY

Siriluk P

NEXT CAL DATE

09/10/26

Submitted by : ALS Laboratory Group (Thailand) Co.,Ltd.
104 Phatthanakan 40, Phatthanakan Rd.,
Khwaeng Phatthanakan, Khet Suan Luang,
Bangkok 10250 Thailand

Location : Organic Preparation Lab

Received Order : 08 October 2025

Calibration Date : 09 October 2025

Ambient Temperature : (26 ± 10) °C

Relative Humidity : (50 ± 30) %

AC Line Voltage : (220 ± 22) V

Calibrated by : Kunchit Promprat

Kunchit Promprat

Approved by :

Approved Signatory

() Chakrit Waewwanjua

() Ponpan Paipim

(✓) Suwit Imjai

Issue Date : 28 October 2025

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.



Equipment : Water Bath
Condition As-Received : Used Item
Reference : 2510-0042OC-13

Cert. No.: 25TM528
Page : 2 of 3

Procedure Used :-

Calibration were conducted using in-house calibration procedure CP-OT04 Based on ASTM E715 according to direct measurement method with Data Acquisition which connected with Industrial Platinum Resistance Thermometer (IPRT).

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

<u>Instrument</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Traceable</u>	<u>Due Date</u>
1) Data Acquisition	MY58041391	25LM20	TPA	08 Feb 2026

2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This measurement result is traceable to the International System of Unit maintained through :


Remark : TPA : Technology Promotion Association (Thailand - Japan)

Result of Calibration :- (*) Without Adjustment

Function of UUC* : Temperature Source

Heat transfer medium used : Water

	<u>Environmental</u>		<u>AC Voltage Supply</u> (Volt)
	(°C)	(%R.H.)	
Beginning of Calibration	24	63	224
Finished of Calibration	24	58	224

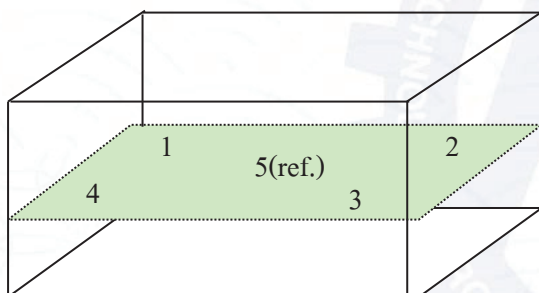

Front

<u>Position :</u>	<u>Ref. Std. ID No.:</u>
1	70RC143
2	70RC144
3	70RC145
4	70RC146
5(ref.)	70RC147



Equipment : Water Bath
Condition As-Received : Used Item
Reference : 2510-0042OC-13
Result of Calibration :- (*) Without Adjustment
Function of UUC* : Temperature Source

Cert. No.: 25TM528

Page : 3 of 3

Calibration point (°C)	UUC* Setting (°C)	UUC* Reading (°C)	Average* Standard Reading (°C)					Uncertainty (± °C)
			Position					
			1	2	3	4	5 (ref.)	
85.0	85.0	85.0	84.863	84.748	84.869	84.990	84.966	0.21

Calibration point (°C)	Uniformity (°C)	Stability (± °C)	Coverage Factor <i>k</i>
85.0	0.33	0.12	2

Average* : The average of 30 values in each position.

Uniformity : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.

Stability : One-half of the greatest maximum difference of measured temperature at any one probe.

UUC* : Unit Under Calibration

Note : The reported uncertainty of measurement was included stability and excluded uniformity.

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

Certificate No. T251785

Page 1 of 3

Certificate of Calibration**Equipment : Chamber (Oven)****Manufacturer : Memmert****Model : UF110****Serial No. : B423.1549****Customer Code : BKK_EN0425****ID No. : T4671A5****Customer : ALS Laboratory Group (Thailand) Co.,Ltd.**

104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan,

Khet Suan Luang, Bangkok 10250

Customer Location : Oven Room**Date of Receipt : 1 October 2025****Calibrated By : Sujjar Naknakred (Site Calibration Manager)****Approved By : Don Zai Boonchai Suriyawong (Site Calibration Manager)****Date of Issue : 10 OCT 2025**

REVIEW BY	<u>finda k</u>
APPROVED BY	<u>Siriluk P.</u>
NEXT CAL. DATE	<u>06/10/26</u>

The uncertainties are for a confidence probability of approximately 95%.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standard laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Metrological Center.

Certificate No. T251785

Page 2 of 3

Calibration Report

Equipment : Chamber (Oven)
Date of Calibration : 6 October 2025
Environment : Temperature : 24.4-25.8 °C
Line Voltage : 220.5-225.2 V
Relative Humidity : 55 - 65 %RH

Condition of this results of calibration :

1. This equipment was calibrated by insert nine resistance thermometer detectors into its chamber , the other one resistance thermometer detector use for ambient temperature measurement . The calibration was done in according to WI-T20 (based on ASTM E145-94 (Reapproved 2019) and AS2853-1986).

All data show below were final values and the initial data from customer request . The temperature scale used was based on ITS - 90 .

2. Reference Standard Instrument :

Instrument	Model	Instrument No.	Certificate No.	Due Date
RTD	100 ohm	23-(CH1-10)	T250314	6 April 2026
DATA LOGGER	34970A	T195	T250314	6 April 2026

3. This certificate is traceable to :

National Institute of Metrology (Thailand) through Metrological Center (NSC-TISI-TIS 17025 CALIBRATION 0244.

4. Condition of calibrated item : good

Equipment Description :

Time Constant 2 Hour 14 Minute At 104 °C
Fresh Air Damper ☒ Open ☒ Min ☐ Medium ☐ Max
☐ Close
☐ Not Available

5. Adjustment :

() without adjustment


(X) after adjustment

Approved By. Donkai

Certificate No. T251785

Page 3 of 3

Calibration Report

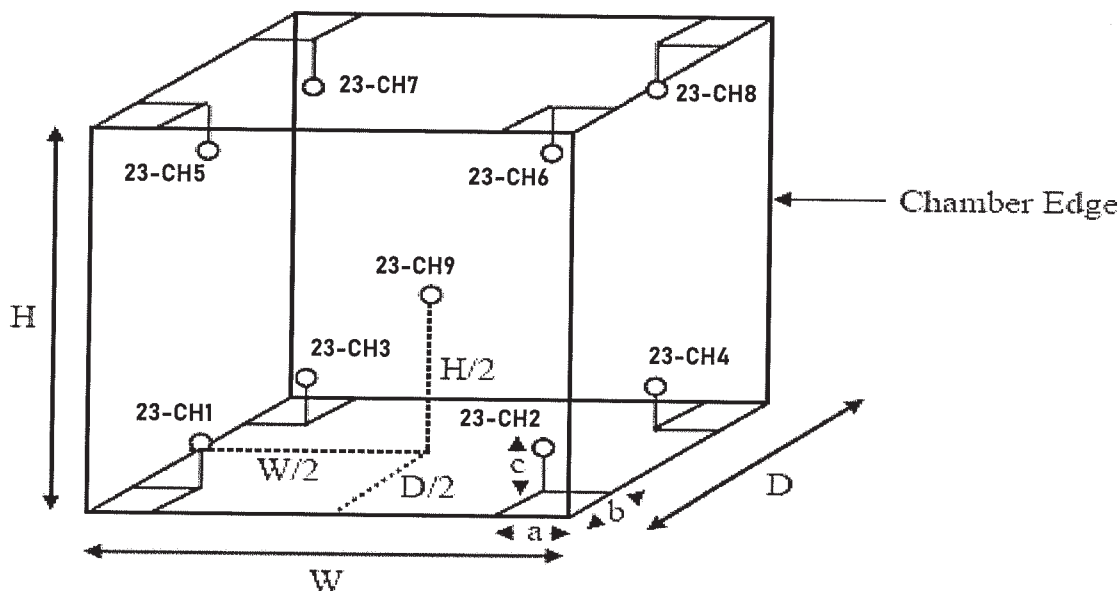

Remark : Internal Dimensions of Chamber : W (Width) = 56 cm. , H (Height) = 48 cm. and D (Depth) = 40 cm.
 Size of Installed Standard sensor number 23-CH1 to number 23-CH8 : a = 5 cm. , b = 5 cm. and c = 5 cm.
 Size of Installed Standard sensor number 23-CH9 : W/2 = 56 cm./2 , H/2 = 48 cm./2 and D/2 = 40cm./2

Measurement Results

Average Standard Reading at each position (°C)									
Calibration Point	23-CH1	23-CH2	23-CH3	23-CH4	23-CH5	23-CH6	23-CH7	23-CH8	23-CH9
104	104.13	103.54	103.92	104.37	104.40	104.51	104.18	103.86	103.80
180	180.05	179.82	179.64	179.52	181.20	180.29	180.19	179.35	179.89

Chamber (Oven)			Temperature Distribution				
Setting °C	Reading (°C)		Average (°C)	Stability (± °C)	Uniformity (°C)	Uncertainty (± °C)	Coverage Factor k
	Min , Max	Average					
104.0	-	104.0	104.08	0.28	0.87	0.45	2.00
180.0	180.0 , 180.1	180.0	179.99	0.37	1.49	0.61	2.00

* The quoted uncertainty exclude "uniformity"

The calibration result apply only the above calibrated item.

The result of test was found accurate as shown on date and place of test only.

The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor k which for a t-distribution, providing a level of confidence of approximately 95 % .

End of Certificate.

Approved By. 

Certificate of Calibration

Customer

Name : ALS Laboratory Group Thailand Co., Ltd.
Address : 104 Soi Phatthanakan 40, Phatthanakan Road, Suan Luang,
Bangkok 10250

Certificate No : 24-AFM-179

Request No : Req-2024-1987

Unit Under Calibration Details

Measurement Item : Air Flow Meter
Manufacturer : MesaLabs Accuracy : 1% of Reading
Model : Defender 510-M Sensor Model : -
Serial Number : 151114 Sensor Serial Number : -
ID : BKK_FS0614 Instrument Status : Used
Location of Calibration : LAB 4 AIR VELOCITY METER

Calibration Environment and Details

Temperature : 23 °C ± 3 °C
Humidity : 55 %RH ± 20 %RH
Barometric Pressure : 1013 hPa ± 10 hPa
Received Date : 30 August 2024
Calibration Date : 9 September 2024
Calibration Procedure : In-house method CP-AFM-01 by Comparison technique with Standard Primary Flow Calibrator



Reference Standard	Model	Serial Number	Traceable	Due Calibration
Air Flow Meter	Gilibrator 3 Low flow	18501010006	Sensidyne	6 August 2025
Air Flow Meter	Gilibrator 3 Standard flow	19031011003	Sensidyne	2 August 2025
Temperature meter	GT 11	08000057	Qreborn	1 March 2025
Pressure meter	CPG2400	41000KDU/651882	TPA	9 November 2024

Traceability :

This Certificate is traceable to SI Unit through Sensidyne A2LA Accreditation No. 3943.01

Note :

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor $k = 2$, providing a level of confidence approximately 95 %.

Calibration By : [Signature]
Mr. Noppadon Luangart
Service Calibration Engineer

Approved By : [Signature]
Mr. Pacit Mathavorn
Calibration Engineer Supervisor

Issue Date : 9 September 2024

Certificate No : 24-AFM-179

Request No : Req-2024-1987

Result of Calibration : Without Adjustment

Temperature (°C)	Pressure (kPa)	STD (cc/min)	UUC (cc/min)	Error (cc/min)	Uncertainty (cc/min)	MPE (cc/min)	Result
24.70	100.95	100	100.41	0.4	2.8	1.0	N/A
24.90	100.90	502	500.47	-1.5	7.1	5.0	N/A
24.90	100.97	1003	1001.3	-2	14	10.0	N/A
25.00	100.92	2014	2009.9	-4	29	20.1	N/A
25.20	101.03	3043	3058.3	15	44	30.4	N/A
25.30	101.10	4043	4005.1	-38	57	40.4	N/A
25.50	101.15	5052	5003.9	-48	74	50.5	N/A

Note

STD : Standard UUC : Unit Under Calibration

- UUC Reference Condition : At atmospheric pressure and room temperature condition

- Flow Rate was corrected for non-standard operating condition by using equation :

$$Q_{meas} = Q_{ref} \times \frac{P_{ref}}{P_{meas}} \times \frac{T_{meas}}{T_{ref}}$$

where Q = Flow Rate P = Absolute Pressure T = Absolute Temperature

Meas = Measurement Condition ref = Standard Condition

* Indicates non accredited

MPE = Maximum Permissible Error (Specified in Manufacturer's Specifications)

N/A = Not Available, Customer does not require a statement of conformity.

Certificate No : 24-AFM-179

Request No : Req-2024-1987

Decision Rule for Statements of Conformity


The standard decision rule employed for the statements of conformity to each calibration result will be applied using ILAC-G8:09/2019; Guidelines on the Reporting of Compliance with Specification as following Fig. and statements

Pass = The measurement result plus the expanded uncertainty with a 95% coverage probability were within the limit.

Pass¹ = The measurement result was within the limit. However, a portion of the expanded uncertainty of measurement at 95% exceeds the limit.

Fail¹ = The measurement result was out of the limit. However, a portion of the expanded uncertainty of measurement at 95% is within the limit.

Fail = The measurement result plus the expanded uncertainty with a 95% coverage probability were outside the limit.

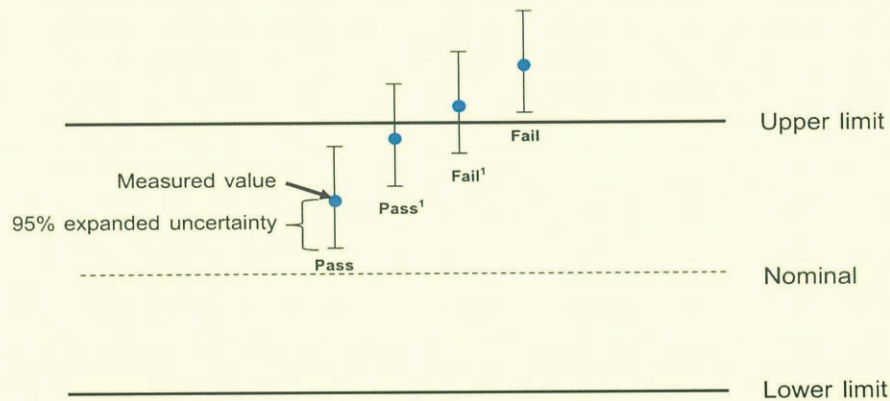

End of Certificate

Certificate of Calibration

Customer

Name : ALS Laboratory Group Thailand Co., Ltd.
Address : 104 Soi Phatthanakan 40, Phatthanakan Road, Suan Luang,
Bangkok 10250

Certificate No : 24-AFM-177

Request No : Req-2024-1862

Unit Under Calibration Details

Measurement Item : Air Flow Meter
Manufacturer : Bios
Model : Defender 510-L
Serial Number : 130026
ID : BKK_FS0619

Accuracy : 1% of Reading

Sensor Model : -

Sensor Serial Number : -

Instrument Status : Used

Location of Calibration : LAB 4 AIR VELOCITY METER

Calibration Environment and Details

Temperature : 23 °C ± 3 °C
Humidity : 55 %RH ± 20 %RH
Barometric Pressure : 1013 hPa ± 10 hPa
Received Date : 22 August 2024
Calibration Date : 9 September 2024
Calibration Procedure : In-house method CP-AFM-01 by Comparison technique with Standard Primary Flow Calibrator

REVIEW BY	<i>Marathon P</i>
APPROVED BY	<i>[Signature]</i>
NEXT CAL. DATE	9/9/26

Reference Standard	Model	Serial Number	Traceable	Due Calibration
Air Flow Meter	Gilibrator 3 Low flow	18501010006	Sensidyne	6 August 2025
Air Flow Meter	Gilibrator 3 Standard flow	19031011003	Sensidyne	2 August 2025
Temperature meter	GT 11	08000057	Qreborn	1 March 2025
Pressure meter	CPG2400	41000KDU/651882	TPA	9 November 2024

Traceability :

This Certificate is traceable to SI Unit through Sensidyne A2LA Accreditation No. 3943.01

Note :

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor $k = 2$, providing a level of confidence approximately 95 %.

Calibration By : *[Signature]*
Mr. Noppadon Luangart
Service Calibration Engineer

Approved By : *[Signature]*
Mr. Pacit Mathavorn
Calibration Engineer Supervisor

Issue Date : 9 September 2024

Certificate No : 24-AFM-177

Request No : Req-2024-1862

Result of Calibration : Without Adjustment

Temperature (°C)	Pressure (kPa)	STD (cc/min)	UUC (cc/min)	Error (cc/min)	Uncertainty (cc/min)	MPE (cc/min)	Result
24.70	100.92	20	20.192	0.2	1.3	0.2	N/A
24.70	100.90	100	99.923	-0.1	2.8	1.0	N/A
24.70	100.94	201	200.7	-0.3	5.6	2.0	N/A
24.70	100.97	298	300.1	2.1	8.4	3.0	N/A
24.70	100.99	403	399.1	-4	11	4.0	N/A
24.80	101.05	482	477.6	-4.4	6.9	4.8	N/A

Note

STD : Standard UUC : Unit Under Calibration

- UUC Reference Condition : At atmospheric pressure and room temperature condition

- Flow Rate was corrected for non-standard operating condition by using equation :

$$Q_{meas} = Q_{ref} \times \frac{P_{ref}}{P_{meas}} \times \frac{T_{meas}}{T_{ref}}$$

where Q = Flow Rate P = Absolute Pressure T = Absolute Temperature

Meas = Measurement Condition ref = Standard Condition

* Indicates non accredited

MPE = Maximum Permissible Error (Specified in Manufacturer's Specifications)

N/A = Not Available, Customer does not require a statement of conformity.

Certificate No : 24-AFM-177

Request No : Req-2024-1862

Decision Rule for Statements of Conformity


The standard decision rule employed for the statements of conformity to each calibration result will be applied using ILAC-G8:09/2019; Guidelines on the Reporting of Compliance with Specification as following Fig. and statements

Pass = The measurement result plus the expanded uncertainty with a 95% coverage probability were within the limit.

Pass¹ = The measurement result was within the limit. However, a portion of the expanded uncertainty of measurement at 95% exceeds the limit.

Fail¹ = The measurement result was out of the limit. However, a portion of the expanded uncertainty of measurement at 95% is within the limit.

Fail = The measurement result plus the expanded uncertainty with a 95% coverage probability were outside the limit.

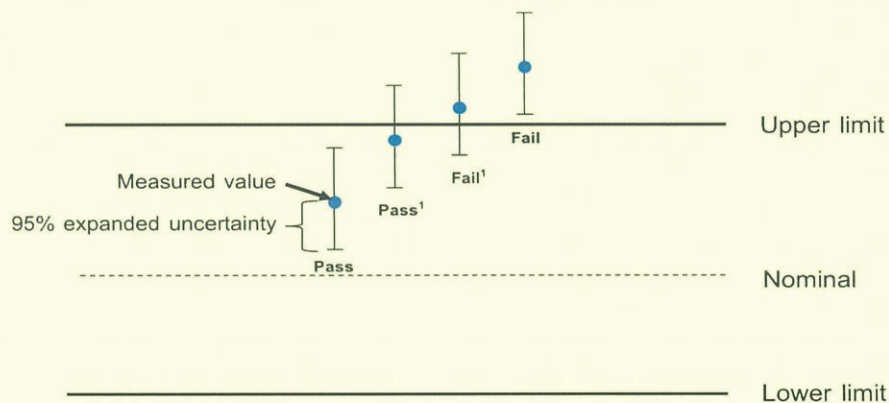

End of Certificate



Certificate of Calibration

Certificate No. C-010925-SGK_FS0153

Air Sampling Pump Detail

Equipment name : Personal Air Sampling Pump
Brand : Gilian
Model/Type : GilAir Plus

Equipment ID : SGK_FS0153
Serial No. : 20170810061
Calibration Date : 01-Sep-25
Next calibration date : 01-Dec-25

Reference Standard Low Flow Meter

Equipment name : Air Flow Meter
Brand : MesaLabs
Model/Type : Defender 510-L

Equipment ID : BKK_FS0619
Serial No. : 130026
Calibration Date : 9-Sep-24
Due Date : 9-Sep-25

Reference Standard High Flow Meter

Equipment name : Air Flow Meter
Brand : MesaLabs
Model/Type : Defender 510-M

Equipment ID : BKK_FS0614
Serial No. : 151114
Calibration Date : 9-Sep-24
Due Date : 9-Sep-25

Calibration Data

Air Sampling Pump setting (cc/min)	Reference Std. Flow Reading (cc/min)			Avg. (cc/min)	%Error acceptance	Acceptable range (cc/min)	Evaluation (Pass/ Fail)
	1	2	3				
Low Flow							
20	19.7	19.9	19.6	19.7	5%	19 - 21	Passed
50	49.8	48.9	49.3	49.3	5%	48 - 53	Passed
100	99.8	99.7	99.9	99.8	5%	95 - 105	Passed
200	200.2	201.3	200.6	200.7	5%	190 - 210	Passed
High Flow							
500	500.9	502.1	499.2	500.7	3%	485 - 515	Passed
1000	1000.9	1001.3	1001.2	1001.1	3%	970 - 1030	Passed
2000	2000.6	1999.4	1996.5	1998.8	3%	1940 - 2060	Passed
2500	2500.7	2501.6	2499.2	2500.5	3%	2425 - 2575	Passed

----- END OF REPORT -----

Calibrated By: 

(Mr. Apiwat Chanta)

SGK Field Services Scientist (2)

Issue date : 02-Sep-25

Approved By: 

(Mr. Supot Salamteh)

Field Services Section Head



Certificate of Calibration

Certificate No. C-010925-SGK_FS0155

Air Sampling Pump Detail

Equipment name : Personal Air Sampling Pump
Brand : Gilian
Model/Type : GilAir PlusEquipment ID : SGK_FS0155
Serial No. : 20170810063
Calibration Date : 01-Sep-25
Next calibration date : 01-Dec-25

Reference Standard Low Flow Meter

Equipment name : Air Flow Meter
Brand : MesaLabs
Model/Type : Defender 510-LEquipment ID : BKK_FS0619
Serial No. : 130026
Calibration Date : 9-Sep-24
Due Date : 9-Sep-25

Reference Standard High Flow Meter

Equipment name : Air Flow Meter
Brand : MesaLabs
Model/Type : Defender 510-MEquipment ID : BKK_FS0614
Serial No. : 151114
Calibration Date : 9-Sep-24
Due Date : 9-Sep-25

Calibration Data

Air Sampling Pump setting (cc/min)	Reference Std. Flow Reading (cc/min)			Avg. (cc/min)	%Error acceptance	Acceptable range (cc/min)	Evaluation (Pass/ Fail)
	1	2	3				
Low Flow							
20	19.9	19.4	20.2	19.8	5%	19 - 21	Passed
50	49.5	49.9	50.1	49.8	5%	48 - 53	Passed
100	97.4	96.2	97.0	96.9	5%	95 - 105	Passed
200	199.3	198.5	200.1	199.3	5%	190 - 210	Passed
High Flow							
500	505.4	503.2	502.6	503.7	3%	485 - 515	Passed
1000	1005.6	1004.3	1006.2	1005.4	3%	970 - 1030	Passed
2000	1998.3	2000.1	2002.1	2000.2	3%	1940 - 2060	Passed
2500	2496.7	2502.3	2501.3	2500.1	3%	2425 - 2575	Passed

----- END OF REPORT -----

Calibrated By: 

(Mr. Apiwat Chanta)

SGK Field Services Scientist (2)

Issue date : 02-Sep-25

Approved By: 

(Mr. Supot Salamteh)

Field Services Section Head



Certificate of Calibration

Certificate No. C-010925-SGK_FS0156

Air Sampling Pump Detail

Equipment name : Personal Air Sampling Pump
Brand : Gilian
Model/Type : GilAir PlusEquipment ID : SGK_FS0156
Serial No. : 20190710133
Calibration Date : 01-Sep-25
Next calibration date : 01-Dec-25

Reference Standard Low Flow Meter

Equipment name : Air Flow Meter
Brand : MesaLabs
Model/Type : Defender 510-LEquipment ID : BKK_FS0619
Serial No. : 130026
Calibration Date : 9-Sep-24
Due Date : 9-Sep-25


Reference Standard High Flow Meter

Equipment name : Air Flow Meter
Brand : MesaLabs
Model/Type : Defender 510-MEquipment ID : BKK_FS0614
Serial No. : 151114
Calibration Date : 9-Sep-24
Due Date : 9-Sep-25

Calibration Data

Air Sampling Pump setting (cc/min)	Reference Std. Flow Reading (cc/min)			Avg. (cc/min)	%Error acceptance	Acceptable range (cc/min)	Evaluation (Pass/ Fail)
	1	2	3				
Low Flow							
20	20.0	20.1	20.2	20.1	5%	19 - 21	Passed
50	50.3	50.4	50.1	50.3	5%	48 - 53	Passed
100	100.3	98.2	99.4	99.3	5%	95 - 105	Passed
200	200.3	201.4	200.1	200.6	5%	190 - 210	Passed
High Flow							
500	505.4	499.9	500.4	501.9	3%	485 - 515	Passed
1000	999.6	1001.2	1003.5	1001.4	3%	970 - 1030	Passed
2000	1998.3	2000.1	2002.1	2000.2	3%	1940 - 2060	Passed
2500	2500.3	2502.3	2501.3	2501.3	3%	2425 - 2575	Passed

----- END OF REPORT -----

Calibrated By: 

(Mr. Apiwat Chanta)

SGK Field Services Scientist (2)

Issue date : 02-Sep-25

Approved By: 

(Mr. Supot Salamteh)


Field Services Section Head

TEST REPORT

CUSTOMER NAME	: ALS Laboratory Group (Thailand) Co., Ltd. [บริษัท เอแอลเอส แลборาทอรี กรุ๊ป (ประเทศไทย) จำกัด]						
EQUIPMENT NAME	: THC Analyzer						
MANUFACTURER	: HORIBA	MODEL	: APHA-370	SERIAL NO	: WKJON9M		
STANDARD GAS CONCENTRATION (PPM) (CH4)	: 506.1 PPM			CYLINDER NO	: CC734373		
CYLINDER PRESSURE (psig)	: 1,600 PSI			CERTIFIED DATE	: 12/05/2020		
CERTIFIED BY	: AIRGAS			EXPIRED DATE	: 12/05/2028		

TEST RESULTS

POINT NO	TEST RESULTS						
	IDEAL	ACTUAL CH4	ERROR CH4	%ERROR CH4	ACTUAL THC	ERROR THC	%ERROR THC
ZERO	0.00	0.00	0.00	-	0.00	0.00	-
1	10.00	9.81	-0.19	-1.90	9.95	-0.05	-0.50
2	20.00	19.60	-0.40	-2.00	19.58	-0.42	-2.10
3	30.00	30.03	0.03	0.10	29.91	-0.09	-0.30
4	40.00	40.00	0.00	0.00	40.00	0.00	0.00
AVERAGE (%)				-0.95			-0.73

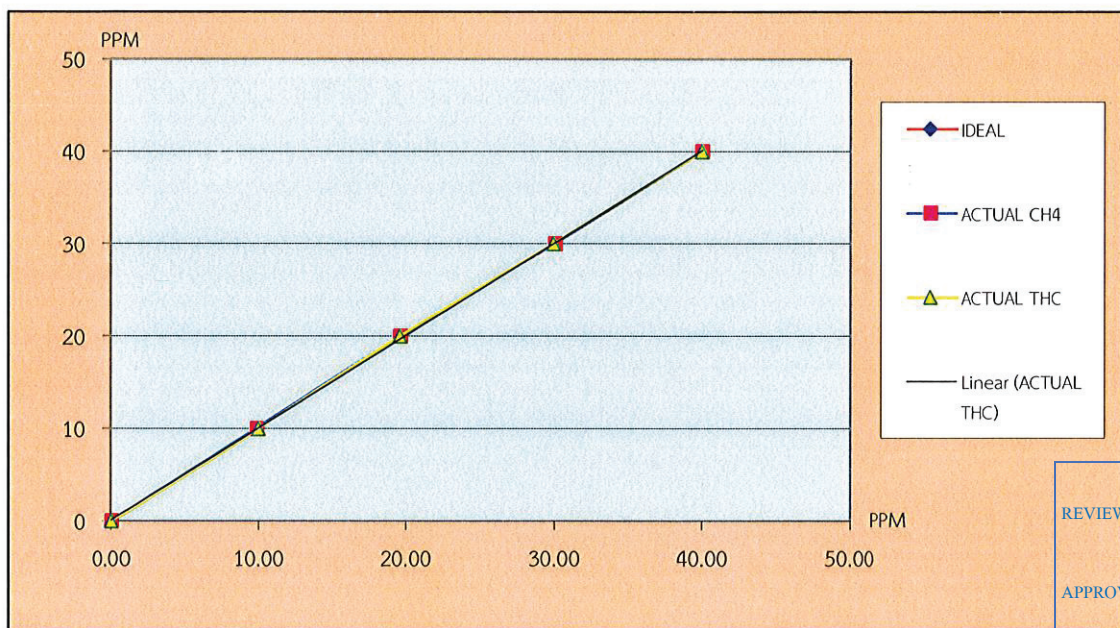

REVIEW BY: Warakorn P.

APPROVED BY: [Signature]

NEXT CAL DATE: 18/06/26

CALIBRATED BY: Warakorn P. DATE: 18/6/68

CHECKED BY: [Signature] DATE: 18/6/68



ต้องการข้อมูลทางด้านเทคนิคเพิ่มเติม : เจ้าหน้าที่ฝ่ายบริการหลังการขาย , โทร 02-868-0812 # 15,16 , E-Mail : Engineer@jiranatee.com
เลขที่ 63/14-15,67/35-36 ถนนเพชรเกษม 7,7/1 แขวงวัดท่าพระ เขตบางกอกใหญ่ กรุงเทพฯ 10600 โทร 02-8680812-13 โทรสาร 02-868-1889

CHECK LIST

CUSTOMER NAME	: ALS Laboratory Group (Thailand) Co., Ltd. [บริษัท เอแอลเอส แลบบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด]		
EQUIPMENT NAME	: THC Analyzer		
MANUFACTURER	: HORIBA	MODEL : APHA-370	SERIAL NO. : WKJON9M

TEST VALUES				
NO.	THC Analyzer (APHA - 370)	UNIT	BEFORE	AFTER
1	Signal (CH4)	mV	1.10	27.50
2	Signal (THC)	mV	0.00	31.60
3	Detector	Temp °C , Standard Value : Ambient temp+(5°Cto15°C)	30.40	48.10
		Pressure kPa , Standard Value : (Ambient/1013x100-20)±4kPa	81.20	81.00
4	Ambient	kPa current atmospheric pressure	101.70	101.60
5	Purifire	°C , Standard Value : 390 °C to 430 °C	30.30	418.70
		kPa , Normal value : 8 kPa to 25 kPa	7.20	7.20
6	NMHC	°C , Standard Value : 230 °C to 260 °C	30.10	244.20
7	DC 24 V	V , Standard Value : 24 V ± 0.5 V	24.90	24.90
8	DC 5 V	V , Standard Value : 5 V ± 0.5 V	4.90	4.90
9	Bypass (Optional)	L/min, Normal value : 0.9 L/min ± 0.3 L/min	-	-
10	Over Flow (Optional)	L/min, Standard Value : 0.8 L/min or More	-	-
11	CH4 Sampling Reading	PPM	1.33	1.95
12	NMHC Sampling Reading	PPM	0.32	0.10
13	THC Sampling Reading	PPM	1.64	2.05
14	Zero Gas CH4/THC	PPM	-0.71/-0.88	0.0/0.0
15	Span Gas	PPM	41.71/41.89	40.0/40.0
G	Gas H2/.....	20 PSI	20	20

Remark : Reference EX-EN-017-56 , Ambient HC Monitor APHA-370 Operation Manual Page #81

Remark : (Ambient temperature = 5°C to 40°C)

อาการที่ตรวจพบ

- Service Maintenance

รายละเอียดการดำเนินการ

- ทำการ Service Maintenance , ทำ Calibration Zero/Span , Multipoint

ผลการดำเนินการ

- เรียบร้อย เครื่องสามารถดำเนินการตรวจวัดได้ตามปกติ

CALIBRATED BY : *สุวิทย์ ขวัญ* *สุวิทย์ ขวัญ*

DATE : *18/6/68*

CHECKED BY : *สุวิทย์ ขวัญ* *สุวิทย์ ขวัญ*

DATE : *18/6/68*



ต้องการข้อมูลทางด้านเทคนิคเพิ่มเติม : เจ้าหน้าที่ฝ่ายบริการหลังการขาย , โทร 02-868-0812 # 15-16 , E-Mail : Engineer@jiranatee.com

เลขที่ 63/14-15,67/35-36 ซอยเพชรเกษม 7,7/1 ถนนเพชรเกษม แขวงวัดท่าพระ เขตบางกอกใหญ่ กรุงเทพฯ 10600 โทร 02-868-0812-13 โทรสาร 02-868-1889

Certificate of System Qualification

GC-OQ + GCMS-OQ

System ID: RYG_EN0136
Organization Name: ALS Laboratory Group (Thailand) Co.Ltd.
Organization Location: 616/10, Moo 5, Tambol Mae Nam Khu, Pluak Daeng, Rayong, 21140, Thailand
Date: July 4, 2025 10:49:05 AM
EQP Name: AgilentRecommended , AgilentRecommended
EQP Revision: GC.02.54, GCMS.02.54
Overall Qualification Status: Pass

REVIEW BY	Chontichai
APPROVED BY	D. Khunkaew
NEXT CAL. DATE	03/01/27

CDS Logon Verification - GC

Logon: chonticha.khunkaew

Overall CDS Logon Verification - GC Test Status

Pass

System Inspection and Basic Safety and Operation

Name: 7890

Setpoint Status: Pass

Overall System Inspection and Basic Safety and Operation Test Status

Pass

Inlet Pressure Accuracy

Name: 7890

Front SSL

Setpoint Status: Pass

	Setpoint	Actual
Inlet Pressure:	25.0 psi	24.9 psi
Accuracy:		0.1 psi
Agilent Recommended:	<=	1.2

Date: July 4, 2025 10:49:05 AM
System ID: RYG_EN0136

Overall Inlet Pressure Accuracy Test Status

Pass

GC Oven Temperature Accuracy

Name: 7890

Setpoint Status: Pass

Zone: Oven

Setpoint/Actual

Temperature: 230.0 231 °C

Accuracy: 1.0 °C

Agilent Recommended: \geq -1.0 % setpoint in K (-5.0 °C)
 \leq 1.0 % setpoint in K (5.0 °C)

Setpoint Status: Pass

Zone: Oven

Setpoint/Actual

Temperature: 100.0 99.8 °C

Accuracy: -0.2 °C

Agilent Recommended: \geq -1.0 % setpoint in K (-3.7 °C)
 \leq 1.0 % setpoint in K (3.7 °C)

Overall GC Oven Temperature Accuracy Test Status

Pass

GC Oven Temperature Stability

Name: 7890

Setpoint Status: Pass

Setpoint/Average

Temperature: 100.0 99.81667 °C

Stability: 0.1 °C

Agilent Recommended: \leq 0.5**Overall GC Oven Temperature Stability Test Status**

Pass

Log Amp

Tested Combination1 Front SSL / External SQ

Name: 5977B

Setpoint Status: Pass

Overall Log Amp Test Status

Pass

RFPA

Tested Combination1 Front SSL / External SQ

Name: 5977B

Setpoint Status: Pass

Amu: 1050 m/z

Drift After Five Minutes:

7 mV

RFPA Voltage:

503 mV

Agilent Recommended:

>= -100 and <= 100

<= 1100

Overall RFPA Test Status

Pass

Tune EI

Tested Combination1 Front SSL / External SQ

Name: 5977B

Setpoint Status: Pass

Filament: 1

Setpoint Status: Pass

Filament: 2

Overall Tune EI Test Status

Pass

Scouting Run

Date: July 4, 2025 10:49:05 AM
System ID: RYG_EN0136

Tested Combination1 Front SSL / External SQ

Manual Injection

Name: Not applicable

Source: EI - Extractor

Setpoint Status: Completed

Injection Volume on Column: 1.0 uL

Overall Scouting Run Status

Completed

Signal to Noise EI

Tested Combination1 Front SSL / External SQ

Name: 5977B

Source: EI - Extractor Filament: 1

Setpoint Status: Pass

Signal to Noise: 1862

Agilent Recommended: \geq 1200

Source: EI - Extractor Filament: 2

Setpoint Status: Pass

Signal to Noise: 1542

Agilent Recommended: \geq 1200

Overall Signal to Noise EI Test Status

Pass

Instrument Details

Purpose

This section describes the as found system configuration.

Details

System

System ID	RYG_EN0136
Manufacturer	Agilent Technologies
Name	7890
Flow Data Input	Manual Data
Temperature Data Input	Manual Data or Other Data Logging

Tested Combination1

Injection Technique	Manual Injection
Inlet	Front
Detector	External
LTM Included?	No

Sampler 1

Manufacturer	Agilent Technologies
Type	Manual Injection
Usage	Sample Injection
Syringe Volume (µL)	10

Mainframe 1

Manufacturer	Agilent Technologies
Name	7890
Model Number	G3442B
Serial Number	CN16463238
Firmware Revision	B.02.04.3
Component ID/Asset No.	081117000236
Oven Type	Standard

Inlet 1

Manufacturer	Agilent Technologies
Name	7890
Type	SSL
Location	Front
Carrier Gas	Helium
Control Type	Electronic Pressure Control (EPC)
Purged Inlet	Yes

Detector 1

Manufacturer	Agilent Technologies
Name	Mass Spectrometer
Type	Mass Spectrometer
Location	External

Mass Spectrometer 1

Manufacturer	Agilent Technologies
Type	SQ
Name	5977B
Model Number	G7077B
Serial Number	US1701M008
Firmware Revision	5977 6.00.34
High Vacuum System	Turbo Pump
Scouting Run Standard	OFN Std
Component ID/Asset No.	081117000236

MS EI Source 1

Manufacturer	Agilent Technologies
Source Type	EI - Extractor
Number of filaments	2

Electronic Signature

Purpose

This signature page was created and published because the ACE sign-off action was executed, which is valid for the entire document, including attachments. The ACE sign-off is an electronic signature that requires two distinct identification components: unique username and personal password. The Agilent representative who has delivered this service understands the meaning and legal status of an electronic signature. As a trained official operator, the Agilent representative has a unique password and logon to access ACE and electronically sign this document. (Other e-signatures can be applied to this document using a Document Content Management or other suitable method defined in your data access and control procedures.)

Details

Full Name of Signer:	Eaknarin Puangsopa
Logged On User Name:	eaknarin_puangsopa@agilent.com
Signature Creation Date:	July 4, 2025
Reason for Signature:	Executed protocol and published this original version of document

ACE Self Qualification Status

The installed version of ACE used to deliver this service passed qualification; the results conform with expected values. The self qualification summary report is available in the session folder location SDS\ClearStore\AceSelfQualification.

Regulatory Disclaimer

This document provides a protocol to verify and record instrument configuration and evidence of proper operation. It has been prepared from our interpretation of applicable regulations as well as industry best practices. The document is designed to provide an important component of a complete compliance package. Validation depends upon many factors and use of this protocol alone does not assure compliance. Agilent Technologies makes no promises or representations as to its sufficiency for any specific regulatory program.

Warranty

Agilent Technologies makes no warranty of any kind to this material, including but not limited to, the implied warranties or merchantability and fitness for a particular purpose. Agilent Technologies shall not be liable for errors contained herein or for incidental or consequential damages in connection with the furnishing, performance, or use of this material.

User Name: eaknarin_puangsopa

System Id: RYG_EN0136

Report Generated by Hostname: AG-5CG22143KR

Print Date: July 4, 2025 10:49:07 AM

ALS_OQ_RYG_EN0136_2025 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
July 3, 2025 12:07:42 PM	Audit	SessionCreated	Session	Host Name: AG-5CG22143KR, Drive Serial Number: 2A984E77
July 3, 2025 12:07:42 PM	start	Configuration	Session	None
July 3, 2025 12:07:42 PM	Audit	Entitlement	Licensing	User is FieldEngineer and does not require an unlock code
July 3, 2025 12:08:37 PM	Audit	EqpLoaded	Session	EQP details for primary technique [Gc] - File path: [ProtocolPacks/Gc/Configurat ions/02.54/Gc.02.54.eqp], EQP File Name: [Gc.02.54.eqp], EQP Name: [AgilentRecommended], Proto col Revision :[Gc.02.54] EQP details for hyphenated technique [GcMs] - File path: [ProtocolPacks/GcMs/Config urations/02.54/GcMs.02.54.e qp], EQP File Name: [GcMs.02.54.eqp], EQP Name: [AgilentRecommended]
July 3, 2025 12:08:41 PM	End	Configuration	Session	None
July 3, 2025 12:08:47 PM	start	Qualification	Session	OQ
July 3, 2025 12:08:48 PM	start	Execution	CDS Logon Verification - GC - 7890: - Qualitative test	None
July 3, 2025 12:12:14 PM	End	Execution	CDS Logon Verification - GC - 7890: - Qualitative test	Run Count : 1

User Name: eaknarin_puangsoa

System Id: RYG_EN0136

Report Generated by Hostname: AG-5CG22143KR

Print Date: July 4, 2025 10:49:07 AM

ALS_OQ_RYG_EN0136_2025 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
July 3, 2025 12:12:17 PM	start	Execution	System Inspection and Basic Safety and Operation - 7890: - Qualitative Test - No setpoints associated	None
July 3, 2025 12:12:35 PM	End	Execution	System Inspection and Basic Safety and Operation - 7890: - Qualitative Test - No setpoints associated	Run Count : 1
July 3, 2025 12:12:38 PM	start	Execution	Inlet Pressure Accuracy - Front SSL: - Pressure Controlled Inlet - S: 25.0 psi - L: <= 1.2 psi	None
July 3, 2025 12:17:02 PM	End	Execution	Inlet Pressure Accuracy - Front SSL: - Pressure Controlled Inlet - S: 25.0 psi - L: <= 1.2 psi	Run Count : 1
July 3, 2025 12:17:04 PM	start	Execution	GC Oven Temperature Accuracy - 7890: - Temperature : Oven - S: 230.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	None
July 3, 2025 12:21:01 PM	Audit	Data	GC Oven Temperature Accuracy - 7890: - Temperature : Oven - S: 230.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	Manual Data Entry
July 3, 2025 12:21:03 PM	End	Execution	GC Oven Temperature Accuracy - 7890: - Temperature : Oven - S: 230.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	Run Count : 1
July 3, 2025 12:21:06 PM	start	Execution	GC Oven Temperature Accuracy - 7890: - Temperature : Oven - S: 100.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	None
July 3, 2025 12:21:22 PM	start	Execution	GC Oven Temperature Accuracy - 7890: - Temperature : Oven - S: 100.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	None

Page 2 / 6

User Name: eaknarin_puangsoa

System Id: RYG_EN0136

Report Generated by Hostname: AG-5CG22143KR

Print Date: July 4, 2025 10:49:07 AM

ALS_OQ_RYG_EN0136_2025 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
July 3, 2025 12:25:15 PM	Audit	Data	GC Oven Temperature Accuracy - 7890: - Temperature : Oven - S: 100.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	Manual Data Entry
July 3, 2025 12:25:17 PM	End	Execution	GC Oven Temperature Accuracy - 7890: - Temperature : Oven - S: 100.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	Run Count : 1
July 3, 2025 12:25:19 PM	start	Execution	GC Oven Temperature Stability - 7890: - Temperature : Oven - S: 100.0°C - L: <= 0.5°C	None
July 3, 2025 12:51:12 PM	Audit	Data	GC Oven Temperature Stability - 7890: - Temperature : Oven - S: 100.0°C - L: <= 0.5°C	Manual Data Entry
July 3, 2025 12:51:15 PM	End	Execution	GC Oven Temperature Stability - 7890: - Temperature : Oven - S: 100.0°C - L: <= 0.5°C	Run Count : 1
July 3, 2025 12:51:24 PM	start	Execution	Log Amp - 5977B SQ: - Source: EI - Extractor	None
July 3, 2025 1:40:17 PM	End	Execution	Log Amp - 5977B SQ: - Source: EI - Extractor	Run Count : 1
July 3, 2025 1:40:19 PM	start	Execution	RFPA - 5977B SQ: - Source: EI - Extractor	None
July 3, 2025 1:48:10 PM	End	Execution	RFPA - 5977B SQ: - Source: EI - Extractor	Run Count : 1
July 3, 2025 1:48:21 PM	start	Execution	Tune EI - 5977B SQ: - Source: EI - Extractor Filament 1 (Qualitative - No setpoints associated)	None
July 3, 2025 2:00:38 PM	End	Execution	Tune EI - 5977B SQ: - Source: EI - Extractor Filament 1 (Qualitative - No setpoints associated)	Run Count : 1

Page 3 / 6

User Name: eaknarin_puangsoipa

System Id: RYG_EN0136

Report Generated by Hostname: AG-5CG22143KR

Print Date: July 4, 2025 10:49:07 AM

ALS_OQ_RYG_EN0136_2025 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
July 3, 2025 2:00:41 PM	start	Execution	Tune EI - 5977B SQ: - Source: - None EI - Extractor Filament 2 (Qualitative - No setpoints associated)	
July 3, 2025 2:11:24 PM	End	Execution	Tune EI - 5977B SQ: - Source: - Run Count : 1 EI - Extractor Filament 2 (Qualitative - No setpoints associated)	
July 3, 2025 2:11:34 PM	start	Execution	Scouting Run - Manual Injection, Front SSL, SQ: - Source: - EI - Extractor- Part of GCMS System Preparation	None
July 3, 2025 2:11:57 PM	Audit	AceClosed	Session	None
July 4, 2025 9:11:18 AM	Audit	AceRestarted	Session	Host Name: AG-5CG22143KR, Drive Serial Number: 2A984E77
July 4, 2025 9:11:22 AM	Audit	SessionReloaded	Session	None
July 4, 2025 9:14:30 AM	start	Qualification	Session	OQ
July 4, 2025 9:14:30 AM	start	Execution	Scouting Run - Manual Injection, Front SSL, SQ: - Source: - EI - Extractor- Part of GCMS System Preparation	None
July 4, 2025 9:30:11 AM	Audit	AceRestarted	Session	Host Name: AG-5CG22143KR, Drive Serial Number: 2A984E77
July 4, 2025 9:30:13 AM	Audit	SessionReloaded	Session	None
July 4, 2025 9:33:02 AM	start	Qualification	Session	OQ
July 4, 2025 9:33:02 AM	start	Execution	Scouting Run - Manual Injection, Front SSL, SQ: - Source: - EI - Extractor- Part of GCMS System Preparation	None

User Name: eaknarin_puangsoa

System Id: RYG_EN0136

Report Generated by Hostname: AG-5CG22143KR

Print Date: July 4, 2025 10:49:07 AM

ALS_OQ_RYG_EN0136_2025 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
July 4, 2025 10:06:33 AM	Audit	Data	Scouting Run - Manual Injection, Front SSL, SQ: - Source: - EI - Extractor- Part of GCMS System Preparation	Manual Data Entry
July 4, 2025 10:06:41 AM	End	Execution	Scouting Run - Manual Injection, Front SSL, SQ: - Source: - EI - Extractor- Part of GCMS System Preparation	Run Count : 1
July 4, 2025 10:06:44 AM	start	Execution	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 1 - L: >= 1200	None
July 4, 2025 10:09:12 AM	Audit	Data	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 1 - L: >= 1200	Manual Data Entry
July 4, 2025 10:09:20 AM	End	Execution	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 1 - L: >= 1200	Run Count : 1
July 4, 2025 10:09:25 AM	start	Execution	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 2 - L: >= 1200	None
July 4, 2025 10:11:28 AM	Audit	Data	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 2 - L: >= 1200	Manual Data Entry
July 4, 2025 10:11:35 AM	End	Execution	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 2 - L: >= 1200	Run Count : 1
July 4, 2025 10:11:38 AM	End	Qualification	Session	OQ

User Name: eaknarin_puangsopa

System Id: RYG_EN0136

Report Generated by Hostname: AG-5CG22143KR

Print Date: July 4, 2025 10:49:07 AM

ALS_OQ_RYG_EN0136_2025 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
July 4, 2025 10:11:38 AM	start	Reporting	Session	None
July 4, 2025 10:34:26 AM	Audit	Reporting	Session	Report Generated : Certificate
July 4, 2025 10:36:02 AM	Audit	Reporting	Session	Report Generated : Report
July 4, 2025 10:39:06 AM	Audit	Reporting	Session	Report Generated : Certificate
July 4, 2025 10:40:07 AM	Audit	Reporting	Session	Report Generated : Report
July 4, 2025 10:47:04 AM	Audit	Reporting	Session	Report Generated : Certificate
July 4, 2025 10:47:40 AM	Audit	Reporting	Session	Report Generated : Report

Certificate Number

CWS-032-67

CERTIFICATE OF CALIBRATION

Page 1 of 2 Pages

MEASUREMENT ITEM : Cup anemometer
MANUFACTURER : Novalynx
MODEL/TYPE : Sensor: WS-02F
Data logger: 110-WS-25DL-D
SERIAL NUMBER : Sensor: WSD-A5791
Data logger: A5791
ID NUMBER : SGK_FS0088
CONDITION AS-RECEIVED : Used item
CUSTOMER : ALS laboratory group (Thailand) Co., Ltd.
104 Phatthanakan 40, Phatthanakan Rd, Khwaeng Suan Luang,
Khet Suan Luang, Bangkok 10250 Thailand.

RECEIVED DATE : 16 Aug 2024
MEASUREMENT DATE : 23 Aug 2024
ISSUE DATE : 23 Aug 2024

ENVIRONMENTAL CONDITIONS:

Ambient condition in the laboratory are as follow:

Temperature : 23.0 ± 3.0 °C
Relative Humidity : 55.0 ± 15.0 %RH
Atmospheric Pressure : 1010 ± 10 hPa

PLACE OF CALIBRATION : Eiffel-type wind tunnel of Jiranatee Associates Co., Ltd.

CALIBRATION CONDITIONS : Wind tunnel cross-section area¹ 900 cm²
Wind direction frontal area² 100 cm²
Diameter of mounting pipe³ - mm
Blockage ratio of test object⁴ 0.111 [-]

Preconditioning : 24 hours at ambient conditions.
Measurement Condition : The average values during measurement are (23.6) °C, (48.4) %RH and (1005.0) hPa.

TABULATION OF RESULTS:

The table on next page give the measured values.

Calibrated by:

- ☒ Mr. Sorawit Thachalad
☐ Miss Jitraporn Lertsomphol



Calibration procedure:

The Cup anemometer was calibrated against Standard air velocity transducer model: 8455-12 and pitot tube with precision differential pressure meter model: DPM2500 in an close test-section of Eiffel-type wind tunnel with 900 cm² cross test section area. The WI-CL-007 based on IEC 61400-12-1, Wind energy generation systems – Part 12-1: Power performance measurements of electricity producing wind turbines, March 2017 was used as a calibration guideline.

Traceability:

This certificate provides a traceability of The measurement to recognized the national standards, and to realization of the international system of units (SI) through the NIMT (National Metrology Institute of Thailand) via Certificate number: MW-0007-24 and MW-0055-23

Uncertainty of Measurement:

The reported uncertainty of measurement is based on the standard uncertainty multiplied by a coverage factor k=2, Which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty has been determined in accordance with the GUM 'Evaluation of measurement data - Guide to the expression of uncertainty in measurement'

REVIEW BY *Marakorn P.*

APPROVED BY *Mr. Parinya Booncharoen*

NEXT CAL. DATE 23/12/26

Approved signatory: *Mr. Parinya Booncharoen*

Mr. Parinya Booncharoen
Calibration Department Manager

Remark:

- ¹ Nozzle cross-section area of the wind tunnel
² Projected cross-section area of the tested object include mounting pipe
³ Diameter of mounting pipe
⁴ Ratio ² to ¹

MEASUREMENT RESULTS⁵

The Cup anemometer, Unit Under Calibration (UUC) was exercise at 10 m/s for 5 minutes prior to calibration being performed. The standard air velocity 0.5 m/s to 5 m/s was calculated by a standard air velocity transducer which was installed 50 mm away from wind tunnel nozzle and installed 40 mm away from top of the test section and the standard air velocity 5 m/s to 30 m/s was calculated by a pitot tube with precision differential pressure meter which was installed 50 mm away from wind tunnel nozzle and installed 40 mm away from top of the test section, UUC was mounted on a round vertical tube of the lower plate at center of test section. The calibration was carried out under both rising and falling air velocity in the range of 1 m/s to 16 m/s at calibration interval of 1 m/s. The results of calibration and associated measurement uncertainties are reported in the table below.


V_{std} ⁶ (m/s)	Temp. wind tunnel (°C)	Temp. room (°C)	V_{UUC} ⁷ (m/s)	Error (m/s)	U ($k=2$) (m/s)
1.047	23.40	23.60	0.9	-0.1	0.31
2.008	23.60	23.60	1.8	-0.2	0.31
2.975	23.24	23.60	2.8	-0.2	0.31
4.042	23.26	23.60	3.8	-0.2	0.31
4.98	23.32	23.60	5.0	0.0	0.31
5.96	23.38	23.60	6.0	0.0	0.31
7.03	23.20	23.60	7.1	0.1	0.31
7.97	23.22	23.60	8.1	0.1	0.31
8.98	23.10	23.60	9.1	0.1	0.31
9.96	23.10	23.60	10.1	0.2	0.31
10.94	23.18	23.60	11.1	0.2	0.31
12.01	23.10	23.60	12.3	0.3	0.31
12.93	23.20	23.60	13.2	0.3	0.31
14.07	23.10	23.60	14.3	0.2	0.31
15.00	23.18	23.60	15.3	0.3	0.31
15.99	23.12	23.60	16.3	0.3	0.31

Remark:

⁵ Calibration results only count for the tested circumstances and environmental conditions during which calibration took place

⁶ Velocity of standard

⁷ Velocity of Unit Under Calibration

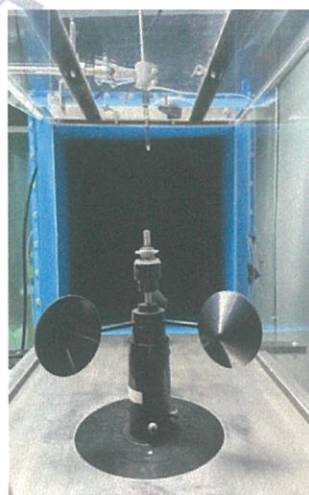PHOTO OF CALIBRATION SET-UP

Calibration set-up of the Cup anemometer calibration in the wind tunnel of Jiranatee Associates Co., Ltd. The Cup anemometer shown may differ from the calibrated one. Remark: The proportion of the set- up is not true to scale due to imaging geometry.



Certificate Number

CWD-032-67

CERTIFICATE OF CALIBRATION

Page 1 of 2 Pages

MEASUREMENT ITEM : Wind Direction Sensor
MANUFACTURER : Novalynx
MODEL/TYPE : Sensor: WS-02F
Data logger: 110-WS-25DL-D
SERIAL NUMBER : Sensor: WSD-A5791
Data logger: A5791
ID NUMBER : SGK_FS0088
CONDITION AS-RECEIVED : Used item
CUSTOMER : ALS laboratory group (Thailand) Co., Ltd.
104 Phatthanakan 40, Phatthanakan Rd, Khwaeng Suan Luang,
Khet Suan Luang, Bangkok 10250 Thailand.

RECEIVED DATE : 16 Aug 2024
MEASUREMENT DATE : 23 Aug 2024
ISSUE DATE : 23 Aug 2024

ENVIRONMENTAL CONDITIONS:

Ambient condition in the laboratory are as follow:

Temperature : 23.0 ± 3.0 °C
Relative Humidity : 55.0 ± 15.0 %RH
Atmospheric Pressure : 1010 ± 10 hPa

PLACE OF CALIBRATION : Eiffel-type wind tunnel of Jiranatee Associates Co., Ltd.

CALIBRATION CONDITION : Wind tunnel cross-section area¹ 900 cm²
Wind direction frontal area² 129 cm²
Diameter of mounting pipe³ - mm
Blockage ratio of test object⁴ 0.143 [-]

Preconditioning : 24 hours at ambient conditions.
Measurement Condition : The average values during measurement are (23.2)°C, (43.7) %RH and (1007.7) hPa.

TABULATION OF RESULTS:

The table on next page give the measured values.

Calibrated by:

- ☒ Mr. Sorawit Thachalad
☐ Miss Jitraporn Lertsomphol



Approved signatory:

Signature

Mr. Parinya Booncharoen
Calibration Department Manager

Remark:

- ¹ Nozzle cross-section area of the wind tunnel
² Projected cross-section area of the tested object include mounting pipe
³ Diameter of mounting pipe
⁴ Ratio ² to ¹

MEASUREMENT RESULTS ⁵

The wind direction sensor was calibrated against standard rotary encoder by comparison method. During calibration, the measurement was carried out at 45° intervals in clockwise and counterclockwise directions after offset adjustment has been made. The flow speed of wind tunnel (usually 5 m/s) is kept constant while the sensor is rotated around its vertical axis. The results of calibration and associated measurement uncertainties are reported in the table below.

Air speed m/s	D^6_{std} Degree (°)	D^7_{uuc} Degree (°)	Error Degree (°)	$U (k=2)$ Degree (°)
5.04	45.000	42	-3	0.80
	90.000	88	-2	0.80
	135.000	135	0	0.80
	180.000	182	2	0.80
	225.000	228	3	0.80
	270.000	273	3	0.80
	315.000	318	3	0.80
	360.000	359	-1	0.80

Remark:

⁵ Calibration results only count for the tested circumstances and environmental conditions during which calibration took place

⁶ Direction of standard

⁷ Direction of Unit Under Calibration

End of Certificate of Calibration





JIRANATEE ASSOCIATES CO.,LTD.

Jiranatee Associates Co.,Ltd
63/14-15, 67/35-36
Petchkasem 7,7/1, Rd. Watthapra, Bangkokyai,
Bangkok 10600 (Thailand)
Tel: +6608680812
Mobile: +66863999453
E-mail: jnac-calibration@jiranatee.com
Web site: www.jiranatee.com

Accredited calibration laboratory
ISO/IEC 17025:2017
NSC-TISI-TIS 17025
CALIBRATION 0367

Pressure measurement laboratory
Calibration services department.



CERTIFICATE OF CALIBRATION

Certificate No. : CPR-012-67

Page 1 of 2 Pages

MEASUREMENT ITEM : Digital barometer
MANUFACTURER : Novalynx
MODEL/TYPE : Sensor: 110-WS-25BP
Data logger: 110-WS-25DL-D
SERIAL NUMBER : Sensor: BP-A5791
Data logger: A5791
ID NUMBER : SGK_FS0088
CONDITION AS-RECEIVED : Used item
CUSTOMER : ALS laboratory group (Thailand) Co., Ltd.
104 Phatthanakan 40, Phatthanakan Rd,
Khwaeng Suan Luang, Khet Suan Luang,
Bangkok 10250 Thailand.
RECEIVED DATE : 16 Aug 2024
MEASUREMENT DATE : 23 Aug 2024
ISSUE DATE : 23 Aug 2024

Calibration procedure:

The Digital barometer was calibrated against Digital pressure calibrator. The WI-CL-003 was used as a calibration guideline.

Traceability:

The measurement results are traceable to the international system of units (SI) through the NIMT (National Metrology Institute of Thailand) via Certificate number: MP-0009-24

Uncertainty of Measurement:

The reported uncertainty of measurement is based on the standard uncertainty multiplied by a coverage factor $k=2$, Which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty has been determined in accordance with the GUM 'Evaluation of measurement data - Guide to the expression of uncertainty in measurement'

CONDITION OF THIS RESULT OF CALIBRATION:

1. Reference Standard Instrument:

Instrument	Model	Serial No.	Certificate No.	Due Date
Absolute Pressure Transducer	CPG2500	4100126P	MP-0009-24	27 Dec 2024

1. Calibration effort for calibration sequence C

2. The UUC* was installed in vertical orientation above reference standard instrument and center of UUC* was used as the reference level.

3. Calibration conditions:

4. Condition : ☒ Normal ☐ Abnormal
Pressure transmitting medium : Air
 ρ_{Fl} (20°C, 1 bar) : 1.19 kg/m³
 H_{amb} : (55±15) %
 t_{amb} : (23±3) °C
 p_{amb} : (1010±10) mbar

5. The certificate is valid only to the item calibrated on date and place of calibration

Calibrated by:

☒ Mr. Sorawit Thachalad
☐ Miss Jitraporn Lertsomphol



Approved signatory:

Mr. Parinya Booncharoen
Calibration Department Manager



JIRANATEE ASSOCIATES CO.,LTD.

Jiranatee Associates Co.,Ltd.
63/14-15, 67/35-36
Petchkasem 7,7/1, Rd.Watthapra, Bangkokyai,
Bangkok10600(Thailand)
Tel: +6608680812
Mobile: +66863999453
E-mail: jnac-calibration@jiranatee.com
Web site: www.jiranatee.com

Accredited calibration laboratory
ISO/IEC 17025:2017
NSC-TISI-TIS 17025
CALIBRATION 0367

Pressure measurement laboratory
Calibration services department.



CERTIFICATE OF CALIBRATION

Certificate No. : CPR-012-67

Page 2 of 2 Pages

MEASUREMENT RESULTS : ☐ Without adjustment ☒ With adjustment

CALIBRATION IN THE RANGE OF : 950 mbar to 1050 mbar

The results of calibration and associated measurement uncertainties are reported in the table below.

STD (mbar)	UUC* (mbar)	Error (mbar)	Uncertainty (k=2) (mbar)
950.03	951.6	1.6	0.37
970.01	971.3	1.3	0.37
989.96	990.8	0.9	0.39
1010.03	1010.4	0.4	0.37
1030.02	1030.0	0.0	0.40
1050.02	1049.4	-0.6	0.40

Note: UUC* Unit Under Calibration

: To convert the result in report unit to Pa should be multiply by 100

End of certificate



Certificate Number

CWS-022-67

CERTIFICATE OF CALIBRATION

Page 1 of 2 Pages

MEASUREMENT ITEM : Cup anemometer
MANUFACTURER : Novalynx
MODEL/TYPE : Sensor: WS-02F
Data logger: 200-WS-25LB
SERIAL NUMBER : Sensor: WSD-A5192
Data logger: A5192
ID NUMBER : SGK_FS0035
CONDITION AS-RECEIVED : Used item
CUSTOMER : ALS laboratory group (Thailand) Co., Ltd.
104 Phatthanakan 40, Phatthanakan Rd, Khwaeng Suan Luang,
Khet Suan Luang, Bangkok 10250 Thailand.

RECEIVED DATE : 27 Jun 2024
MEASUREMENT DATE : 03 Jul 2024
ISSUE DATE : 03 Jul 2024

ENVIRONMENTAL CONDITIONS:

Ambient condition in the laboratory are as follow:

Temperature : 23.0 ± 3.0 °C
Relative Humidity : 55.0 ± 15.0 %RH
Atmospheric Pressure : 1010 ± 10 hPa

PLACE OF CALIBRATION : Eiffel-type wind tunnel of Jiranatee Associates Co., Ltd.

CALIBRATION CONDITIONS : Wind tunnel cross-section area¹ 900 cm²
Wind direction frontal area² 100 cm²
Diameter of mounting pipe³ - mm
Blockage ratio of test object⁴ 0.111 [-]

Preconditioning : 24 hours at ambient conditions.
Measurement Condition : The average values during measurement are (24.1) °C, (48.8) %RH and (1005.7) hPa.

TABULATION OF RESULTS:

The table on next page give the measured values.

Calibrated by:

- ☒ Mr. Sorawit Thachalad
☐ Miss Jitraporn Lertsomphol



Calibration procedure:

The Cup anemometer was calibrated against Standard air velocity transducer model: 8455-12 and pitot tube with precision differential pressure meter model: DPM2500 in an close test-section of Eiffel-type wind tunnel with 900 cm² cross test section area. The WI-CL-007 based on IEC 61400-12-1, Wind energy generation systems – Part 12-1: Power performance measurements of electricity producing wind turbines, March 2017 was used as a calibration guideline.

Traceability:

This certificate provides a traceability of The measurement to recognized the national standards, and to realization of the international system of units (SI) through the NIMT (National Metrology Institute of Thailand) via Certificate number: MW-0007-24 and MW-0055-23

Uncertainty of Measurement:

The reported uncertainty of measurement is based on the standard uncertainty multiplied by a coverage factor $k=2$, Which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty has been determined in accordance with the GUM 'Evaluation of measurement data - Guide to the expression of uncertainty in measurement'

REVIEW BY

APPROVED BY

NEXT CAL. DATE

Approved signatory:

Mr. Parinya Booncharoen
Calibration Department Manager

Remark:

- ¹ Nozzle cross-section area of the wind tunnel
² Projected cross-section area of the tested object include mounting pipe
³ Diameter of mounting pipe
⁴ Ratio ² to ¹

MEASUREMENT RESULTS ⁵

The Cup anemometer, Unit Under Calibration (UUC) was exercised at 10 m/s for 5 minutes prior to calibration being performed. The standard air velocity 0.5 m/s to 5 m/s was calculated by a standard air velocity transducer which was installed 50 mm away from wind tunnel nozzle and installed 40 mm away from top of the test section and the standard air velocity 5 m/s to 30 m/s was calculated by a pitot tube with precision differential pressure meter which was installed 50 mm away from wind tunnel nozzle and installed 40 mm away from top of the test section, UUC was mounted on a round vertical tube of the lower plate at center of test section. The calibration was carried out under both rising and falling air velocity in the range of 1 m/s to 16 m/s at calibration interval of 1 m/s. The results of calibration and associated measurement uncertainties are reported in the table below.


V_{std}^6 (m/s)	Temp. wind tunnel (°C)	Temp. room (°C)	V_{UUC}^7 (m/s)	Error (m/s)	$U (k=2)$ (m/s)
1.005	24.10	24.10	0.9	-0.1	0.31
2.008	24.10	24.10	1.8	-0.2	0.31
2.982	24.10	24.10	3.0	0.0	0.31
4.099	24.10	24.10	3.9	-0.2	0.31
4.98	24.00	24.10	5.1	0.1	0.31
5.99	24.26	24.10	6.1	0.1	0.31
7.04	23.86	24.10	7.2	0.2	0.31
7.99	24.06	24.10	8.1	0.1	0.31
9.04	23.62	24.10	9.2	0.2	0.31
10.00	23.86	24.10	10.2	0.2	0.31
10.99	23.60	24.10	11.3	0.3	0.31
11.99	23.70	24.10	12.2	0.2	0.31
12.99	23.68	24.10	13.3	0.3	0.31
14.03	23.66	24.10	14.4	0.4	0.31
15.05	23.60	24.10	15.4	0.4	0.31
15.98	23.70	24.10	16.4	0.4	0.31

Remark:

⁵ Calibration results only count for the tested circumstances and environmental conditions during which calibration took place

⁶ Velocity of standard

⁷ Velocity of Unit Under Calibration

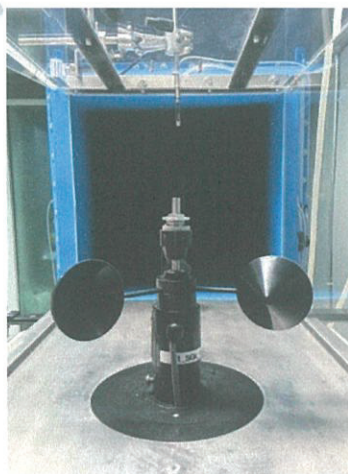PHOTO OF CALIBRATION SET-UP

Calibration set-up of the Cup anemometer calibration in the wind tunnel of Jiranatee Associates Co., Ltd. The Cup anemometer shown may differ from the calibrated one. Remark: The proportion of the set-up is not true to scale due to imaging geometry.



Certificate Number

CWD-022-67

CERTIFICATE OF CALIBRATION

Page 1 of 2 Pages

MEASUREMENT ITEM : Wind Direction Sensor
MANUFACTURER : Novalynx
MODEL/TYPE : Sensor: WS-02F
Data logger: 200-WS-25LB
SERIAL NUMBER : Sensor: WSD-A5192
Data logger: A5192
ID NUMBER : SGK_FS0035
CONDITION AS-RECEIVED : Used item
CUSTOMER : ALS laboratory group (Thailand) Co., Ltd.
104 Phatthanakan 40, Phatthanakan Rd, Khwaeng Suan Luang,
Khet Suan Luang, Bangkok 10250 Thailand.

RECEIVED DATE : 27 Jun 2024
MEASUREMENT DATE : 03 Jul 2024
ISSUE DATE : 03 Jul 2024

ENVIRONMENTAL CONDITIONS:

Ambient condition in the laboratory are as follow:

Temperature	: 23.0 ± 3.0	°C
Relative Humidity	: 55.0 ± 15.0	%RH
Atmospheric Pressure	: 1010 ± 10	hPa

PLACE OF CALIBRATION : Eiffel-type wind tunnel of Jiranatee Associates Co., Ltd.

CALIBRATION CONDITION	: Wind tunnel cross-section area ¹	900	cm ²
	Wind direction frontal area ²	129	cm ²
	Diameter of mounting pipe ³	-	mm
	Blockage ratio of test object ⁴	0.143	[-]

Preconditioning : 24 hours at ambient conditions.
Measurement Condition : The average values during measurement are (23.9)°C, (48.2) %RH and (1008.5) hPa.

TABULATION OF RESULTS:

The table on next page give the measured values.

Calibrated by:

- ☒ Mr. Sorawit Thachalad
☐ Miss Jittraporn Lertsomphol



Approved signatory: _____

Mr. Parinya Booncharoen
Calibration Department Manager

Remark:

- ¹ Nozzle cross-section area of the wind tunnel
² Projected cross-section area of the tested object include mounting pipe
³ Diameter of mounting pipe
⁴ Ratio ² to ¹

Calibration procedure:

The wind direction sensor was calibrated against Standard Rotary Encoder model: AX4009TS-DM04-P3-S-U0 in an close test-section of Eiffel-type wind tunnel with 900 cm² cross test section area. The WI-CL-008 based on IEC 61400-12-1, Wind energy generation systems – Part 12-1: Power performance measurements of electricity producing wind turbines, March 2017 was used as a calibration guideline.

Traceability:

This certificate provides a traceability of The measurement to recognized the national standards, and to realization of the international system of units (SI) through the NIMT (National Metrology Institute of Thailand) via Certificate number: DA-0036-23.

Uncertainty of Measurement:

The reported uncertainty of measurement is based on the standard uncertainty multiplied by a coverage factor k=2, Which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty has been determined in accordance with the GUM 'Evaluation of measurement data - Guide to the expression of uncertainty in measurement'

MEASUREMENT RESULTS ⁵

The wind direction sensor was calibrated against standard rotary encoder by comparison method. During calibration, the measurement was carried out at 45° intervals in clockwise and counterclockwise directions after offset adjustment has been made. The flow speed of wind tunnel (usually 5 m/s) is kept constant while the sensor is rotated around its vertical axis. The results of calibration and associated measurement uncertainties are reported in the table below.

Air speed m/s	D_{std}^6 Degree (°)	D_{uuc}^7 Degree (°)	Error Degree (°)	$U (k=2)$ Degree (°)
5.03	45.000	42	-3	0.80
	90.000	87	-3	0.80
	135.000	132	-3	0.80
	180.000	178	-2	0.80
	225.000	227	2	0.80
	270.000	274	4	0.80
	315.000	319	4	0.80
	360.000	359	-1	0.80

Remark:

⁵ Calibration results only count for the tested circumstances and environmental conditions during which calibration took place

⁶ Direction of standard

⁷ Direction of Unit Under Calibration

End of Certificate of Calibration





JIRANATEE ASSOCIATES CO.,LTD.

Jiranatee Associates Co.,Ltd
63/14-15, 67/35-36
Petchkasem 7,7/1, Rd. Watthapra, Bangkokyai,
Bangkok 10600 (Thailand)
Tel: +6608680812
Mobile: +66863999453
E-mail: jnac-calibration@jiranatee.com
Web site: www.jiranatee.com

Accredited calibration laboratory
ISO/IEC 17025:2017
NSC-TISI-TIS 17025
CALIBRATION 0367

Air speed measurement laboratory
Calibration services department.



Certificate Number

CWS-023-67

CERTIFICATE OF CALIBRATION

Page 1 of 2 Pages

MEASUREMENT ITEM : Cup anemometer
MANUFACTURER : Novalynx
MODEL/TYPE : Sensor: WS-02F
Data logger: 200-WS-25LB
SERIAL NUMBER : Sensor: WSD-A5193
Data logger: A5193
ID NUMBER : SGK_FS0036
CONDITION AS-RECEIVED : Used item
CUSTOMER : ALS laboratory group (Thailand) Co., Ltd.
104 Phatthanakan 40, Phatthanakan Rd, Khwaeng Suan Luang,
Khet Suan Luang, Bangkok 10250 Thailand.

RECEIVED DATE : 27 Jun 2024
MEASUREMENT DATE : 03 Jul 2024
ISSUE DATE : 03 Jul 2024

ENVIRONMENTAL CONDITIONS:

Ambient condition in the laboratory are as follow:

Temperature : 23.0 ± 3.0 °C
Relative Humidity : 55.0 ± 15.0 %RH
Atmospheric Pressure : 1010 ± 10 hPa

PLACE OF CALIBRATION : Eiffel-type wind tunnel of Jiranatee Associates Co., Ltd.

CALIBRATION CONDITIONS : Wind tunnel cross-section area¹ 900 cm²
Wind direction frontal area² 100 cm²
Diameter of mounting pipe³ - mm
Blockage ratio of test object⁴ 0.111 [-]

Preconditioning : 24 hours at ambient conditions.

Measurement Condition : The average values during measurement are (23.9) °C, (50.0) %RH and (1005.3) hPa.

TABULATION OF RESULTS:

The table on next page give the measured values.

Calibrated by:

- ☒ Mr. Sorawit Thachalad
☐ Miss Jitraporn Lertsomphol



Approved signatory:

Mr. Parinya Booncharoen
Calibration Department Manager

Calibration procedure:

The Cup anemometer was calibrated against Standard air velocity transducer model: 8455-12 and pitot tube with precision differential pressure meter model: DPM2500 in an close test-section of Eiffel-type wind tunnel with 900 cm² cross test section area. The WI-CL-007 based on IEC 61400-12-1, Wind energy generation systems – Part 12-1: Power performance measurements of electricity producing wind turbines, March 2017 was used as a calibration guideline.

Traceability:

This certificate provides a traceability of The measurement to recognized the national standards, and to realization of the international system of units (SI) through the NIMT (National Metrology Institute of Thailand) via Certificate number: MW-0007-24 and MW-0055-23

Uncertainty of Measurement:

The reported uncertainty of measurement is based on the standard uncertainty multiplied by a coverage factor $k=2$, Which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty has been determined in accordance with the GUM 'Evaluation of measurement data - Guide to the expression of uncertainty in measurement'

REVIEW BY

APPROVED BY

NEXT CAL DATE

Remark:

- ¹ Nozzle cross-section area of the wind tunnel
² Projected cross-section area of the tested object include mounting pipe
³ Diameter of mounting pipe
⁴ Ratio ² to ¹

THIS CERTIFICATE OF CALIBRATION MAY NOT BE REPRODUCED EXCEPT IN FULL UNLESS PERMISSION FOR REPRODUCTION HAS BEEN OBTAINED IN WRITING FROM THE LABORATORY

MEASUREMENT RESULTS⁵

The Cup anemometer, Unit Under Calibration (UUC) was exercised at 10 m/s for 5 minutes prior to calibration being performed. The standard air velocity 0.5 m/s to 5 m/s was calculated by a standard air velocity transducer which was installed 50 mm away from wind tunnel nozzle and installed 40 mm away from top of the test section and the standard air velocity 5 m/s to 30 m/s was calculated by a pitot tube with precision differential pressure meter which was installed 50 mm away from wind tunnel nozzle and installed 40 mm away from top of the test section, UUC was mounted on a round vertical tube of the lower plate at center of test section. The calibration was carried out under both rising and falling air velocity in the range of 1 m/s to 16 m/s at calibration interval of 1 m/s. The results of calibration and associated measurement uncertainties are reported in the table below.


V_{std}^6 (m/s)	Temp. wind tunnel (°C)	Temp. room (°C)	V_{UUC}^7 (m/s)	Error (m/s)	$U (k=2)$ (m/s)
0.997	24.00	23.85	0.9	-0.1	0.31
2.015	23.70	23.85	1.8	-0.2	0.31
2.990	23.90	23.85	2.9	-0.1	0.31
4.100	23.92	23.85	3.9	-0.2	0.31
4.95	23.80	23.85	5.0	0.0	0.31
5.98	24.00	23.85	6.0	0.0	0.31
7.04	23.62	23.85	7.1	0.0	0.31
7.98	24.00	23.85	8.0	0.0	0.31
9.06	23.62	23.85	9.1	0.0	0.31
10.00	24.04	23.85	10.1	0.1	0.31
11.00	23.66	23.85	11.1	0.1	0.31
12.01	23.90	23.85	12.2	0.1	0.31
13.01	23.70	23.85	13.1	0.1	0.31
14.05	23.80	23.85	14.2	0.2	0.31
15.05	23.70	23.85	15.2	0.1	0.31
16.00	23.76	23.85	16.3	0.3	0.31

Remark:


⁵ Calibration results only count for the tested circumstances and environmental conditions during which calibration took place

⁶ Velocity of standard

⁷ Velocity of Unit Under Calibration

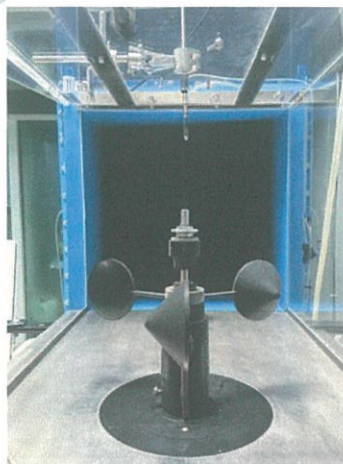PHOTO OF CALIBRATION SET-UP

Calibration set-up of the Cup anemometer calibration in the wind tunnel of Jiranatee Associates Co., Ltd. The Cup anemometer shown may differ from the calibrated one. Remark: The proportion of the set-up is not true to scale due to imaging geometry.

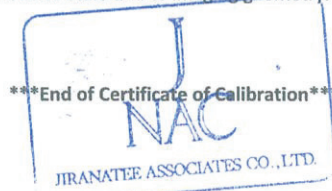

Certificate Number

CWD-023-67

CERTIFICATE OF CALIBRATION

Page 1 of 2 Pages

MEASUREMENT ITEM : Wind Direction Sensor
MANUFACTURER : Novalynx
MODEL/TYPE : Sensor: WS-02F
Data logger: 200-WS-25LB
SERIAL NUMBER : Sensor: WSD-A5193
Data logger: A5193
ID NUMBER : SGK_FS0036
CONDITION AS-RECEIVED : Used item
CUSTOMER : ALS laboratory group (Thailand) Co., Ltd.
104 Phatthanakan 40, Phatthanakan Rd, Khwaeng Suan Luang,
Khet Suan Luang, Bangkok 10250 Thailand.

RECEIVED DATE : 27 Jun 2024
MEASUREMENT DATE : 03 Jul 2024
ISSUE DATE : 03 Jul 2024

ENVIRONMENTAL CONDITIONS:

Ambient condition in the laboratory are as follow:

Temperature	: 23.0 ± 3.0	°C
Relative Humidity	: 55.0 ± 15.0	%RH
Atmospheric Pressure	: 1010 ± 10	hPa

PLACE OF CALIBRATION : Eiffel-type wind tunnel of Jiranatee Associates Co., Ltd.

CALIBRATION CONDITION	: Wind tunnel cross-section area ¹	900	cm ²
	Wind direction frontal area ²	129	cm ²
	Diameter of mounting pipe ³	-	mm
	Blockage ratio of test object ⁴	0.143	[-]

Preconditioning : 24 hours at ambient conditions.

Measurement Condition : The average values during measurement are (23.9)°C, (47.2) %RH and (1008.9) hPa.

TABULATION OF RESULTS:

The table on next page give the measured values.

Calibrated by:

- ☒ Mr. Sorawit Thachalad
☐ Miss Jitraporn Lertsomphol



Approved signatory: _____

Signature

Mr. Parinya Booncharoen
Calibration Department Manager

Remark:

- ¹ Nozzle cross-section area of the wind tunnel
² Projected cross-section area of the tested object include mounting pipe
³ Diameter of mounting pipe
⁴ Ratio ² to ¹

MEASUREMENT RESULTS⁵

The wind direction sensor was calibrated against standard rotary encoder by comparison method. During calibration, the measurement was carried out at 45° intervals in clockwise and counterclockwise directions after offset adjustment has been made. The flow speed of wind tunnel (usually 5 m/s) is kept constant while the sensor is rotated around its vertical axis. The results of calibration and associated measurement uncertainties are reported in the table below.

Air speed m/s	D°_{std} Degree (°)	D°_{uuc} Degree (°)	Error Degree (°)	$U (k=2)$ Degree (°)
5.00	45.000	42	-3	0.80
	90.000	88	-2	0.80
	135.000	132	-3	0.80
	180.000	180	0	0.80
	225.000	227	2	0.80
	270.000	273	3	0.80
	315.000	318	3	0.80
	360.000	359	-1	0.80

Remark:

⁵ Calibration results only count for the tested circumstances and environmental conditions during which calibration took place

⁶ Direction of standard

⁷ Direction of Unit Under Calibration

End of Certificate of Calibration

