ภาคผนวก ง

ใบรับรองการสอบเทียบเครื่องมือ

right solutions.
right partner.

รายการเครื่องมือที่ใช้ในการวิเคราะห์ / ทดสอบ

Sample Name	Parameter	Equipment Name	ID No.	Calibrated Date	Next Cal	Freq. Calibrate (Months)
Ambient	n-Hexane	DRYCAL FLOWMETER	RYG_FS0208	27-Jan-25	26-Jan-26	12
Ambient	n-Hexane	DRYCAL FLOWMETER	BKK_FS0614	9-Sep-24	9-Sep-25	12
Ambient	n-Hexane	DRYCAL FLOWMETER	BKK_FS0614	10-Sep-25	9-Sep-26	12
Ambient	n-Hexane	DRYCAL FLOWMETER	BKK_FS0619	9-Sep-24	9-Sep-25	12
Ambient	n-Hexane	DRYCAL FLOWMETER	BKK_FS0619	10-Sep-25	9-Sep-26	12
Ambient	n-Hexane	GC-FID	BKK_EN0126	22-Oct-24	22-Apr-26	18
Ambient	Ethylene	DRYCAL FLOWMETER	RYG_FS0208	27-Jan-25	26-Jan-26	12
Ambient	Ethylene	DRYCAL FLOWMETER	BKK_FS0614	9-Sep-24	9-Sep-25	12
Ambient	Ethylene	DRYCAL FLOWMETER	BKK_FS0614	10-Sep-25	9-Sep-26	12
Ambient	Ethylene	DRYCAL FLOWMETER	BKK_FS0619	9-Sep-24	9-Sep-25	12
Ambient	Ethylene	DRYCAL FLOWMETER	BKK_FS0619	10-Sep-25	9-Sep-26	12
Ambient	1-Butene	DRYCAL FLOWMETER	RYG_FS0208	27-Jan-25	26-Jan-26	12
Ambient	1-Butene	DRYCAL FLOWMETER	BKK_FS0614	9-Sep-24	9-Sep-25	12
Ambient	1-Butene	DRYCAL FLOWMETER	BKK_FS0614	10-Sep-25	9-Sep-26	12
Ambient	1-Butene	DRYCAL FLOWMETER	BKK_FS0619	9-Sep-24	9-Sep-25	12
Ambient	1-Butene	DRYCAL FLOWMETER	BKK_FS0619	10-Sep-25	9-Sep-26	12
Ambient	1-Hexene	DRYCAL FLOWMETER	RYG_FS0208	27-Jan-25	26-Jan-26	12
Ambient	1-Hexene	DRYCAL FLOWMETER	BKK_FS0614	9-Sep-24	9-Sep-25	12
Ambient	1-Hexene	DRYCAL FLOWMETER	BKK_FS0614	10-Sep-25	9-Sep-26	12
Ambient	1-Hexene	DRYCAL FLOWMETER	BKK_FS0619	9-Sep-24	9-Sep-25	12
Ambient	1-Hexene	DRYCAL FLOWMETER	BKK_FS0619	10-Sep-25	9-Sep-26	12
Ambient	Wind Speed / Wind Direction	Wind Speed / Wind Direction	RYG_FS0329	7-May-25	6-Nov-26	18
Ambient	Wind Speed / Wind Direction	Wind Speed / Wind Direction	RYG_FS0414	29-Oct-24	29-Apr-26	18
Ambient	Wind Speed / Wind Direction	Wind Speed / Wind Direction	BKK_FS0888	1-Aug-25	1-Feb-27	18
Ambient	Wind Speed / Wind Direction	Wind Speed / Wind Direction	RYG_FS0411	29-Oct-24	29-Apr-26	18
Ambient	Wind Speed / Wind Direction	Wind Speed / Wind Direction	BKK_FS0161	6-May-25	6-Nov-26	18
Ambient	Wind Speed / Wind Direction	Wind Speed / Wind Direction	BKK_FS0917	25-Nov-24	25-May-26	18
Workplace	n-Hexane	DRYCAL FLOWMETER	RYG_FS0208	27-Jan-25	26-Jan-26	12
Workplace	n-Hexane	DRYCAL FLOWMETER	BKK_FS0614	9-Sep-24	9-Sep-25	12
Workplace	n-Hexane	DRYCAL FLOWMETER	BKK_FS0614	10-Sep-25	9-Sep-26	12
Workplace	n-Hexane	DRYCAL FLOWMETER	BKK_FS0619	9-Sep-24	9-Sep-25	12
Workplace	n-Hexane	DRYCAL FLOWMETER	BKK_FS0619	10-Sep-25	9-Sep-26	12
Workplace	n-Hexane	GC-FID	BKK_EN0126	22-Oct-24	22-Apr-26	18
Workplace	1-Hexene	DRYCAL FLOWMETER	RYG_FS0208	27-Jan-25	26-Jan-26	12
Workplace	1-Hexene	DRYCAL FLOWMETER	BKK_FS0614	9-Sep-24	9-Sep-25	12
Workplace	1-Hexene	DRYCAL FLOWMETER	BKK_FS0614	10-Sep-25	9-Sep-26	12
Workplace	1-Hexene	DRYCAL FLOWMETER	BKK_FS0619	9-Sep-24	9-Sep-25	12
Workplace	1-Hexene	DRYCAL FLOWMETER	BKK_FS0619	10-Sep-25	9-Sep-26	12
Workplace	Ethylene	DRYCAL FLOWMETER	RYG_FS0208	27-Jan-25	26-Jan-26	12
Workplace	Ethylene	DRYCAL FLOWMETER	BKK_FS0614	9-Sep-24	9-Sep-25	12
Workplace	Ethylene	DRYCAL FLOWMETER	BKK_FS0614	10-Sep-25	9-Sep-26	12
Workplace	Ethylene	DRYCAL FLOWMETER	BKK_FS0619	9-Sep-24	9-Sep-25	12
Workplace	Ethylene	DRYCAL FLOWMETER	BKK_FS0619	10-Sep-25	9-Sep-26	12
Workplace	1-Butene	DRYCAL FLOWMETER	RYG_FS0208	27-Jan-25	26-Jan-26	12
Workplace	1-Butene	DRYCAL FLOWMETER	BKK_FS0614	9-Sep-24	9-Sep-25	12
Workplace	1-Butene	DRYCAL FLOWMETER	BKK_FS0614	10-Sep-25	9-Sep-26	12
Workplace	1-Butene	DRYCAL FLOWMETER	BKK_FS0619	9-Sep-24	9-Sep-25	12
Workplace	1-Butene	DRYCAL FLOWMETER	BKK_FS0619	10-Sep-25	9-Sep-26	12
Noise	Leq 12 hrs	Sound Calibrator	RYG_FS0213	16-Jan-25	16-Jan-26	12
Noise	Leq 12 hrs	Sound Level Meter	RYG_FS0022	19-Mar-25	19-Mar-26	12
Noise	Leq 12 hrs	Sound Level Meter	RYG_FS0024	21-Jan-25	21-Jan-26	12
Noise	Leq 12 hrs	Sound Level Meter	RYG_FS0025	21-Jan-25	21-Jan-26	12
Noise	Leq 12 hrs	Sound Level Meter	RYG_FS0619	21-Jan-25	21-Jan-26	12
Noise	Leq 24 hrs	Sound Calibrator	RYG_FS0496	19-Mar-25	19-Mar-26	12
Noise	Leq 24 hrs	Sound Level Meter	RYG_FS0619	21-Jan-25	21-Jan-26	12
Noise	Leq 24 hrs	Sound Level Meter	RYG_FS0621	27-Jan-25	26-Jan-26	12

right solutions.
right partner.

รายการเครื่องมือที่ใช้ในการวิเคราะห์ / ทดสอบ

Sample Name	Parameter	Equipment Name	ID No.	Calibrated Date	Next Cal	Freq. Calibrate (Months)
Noise	Noise Dose, TWA	Dose Badge Reader	RYG_FS0440	12-Feb-25	11-Feb-26	12
Noise	Noise Dose, TWA	Dosemeter	RYG_FS0033	4-Sep-25	3-Sep-26	12
Noise	Noise Dose, TWA	Dose Badge Reader	RYG_FS0210	12-Feb-25	11-Feb-26	12
Noise	Noise Dose, TWA	Dosemeter	RYG_FS0038	4-Sep-25	3-Sep-26	12
Heat	Heat Stress	Heat Stress Monitor	RYG_FS0580	7-Aug-24	7-Aug-25	12
Heat	Heat Stress	Heat Stress Monitor	RYG_FS0578	6-Aug-24	6-Aug-25	12
Heat	Heat Stress	Heat Stress Monitor	RYG_FS0524	18-Mar-25	17-Mar-26	12
Rayong Lab	pH at 25 ^{o}C	pH Meter	RYG_EN0183	18-Jul-25	18-Jan-27	18
Rayong Lab	BOD	DO meter with Sensor	RYG_EN0032	20-Jan-25	20-Jul-26	18
Rayong Lab	BOD	Incubator	RYG_EN0154	1-Nov-24	1-May-26	18
Rayong Lab	Total Suspended Solids	Electronic Balance	RYG_EN0163	20-Feb-25	20-Feb-26	12
Rayong Lab	Total Suspended Solids	Chamber (Oven)	RYG_EN0012	10-Sep-25	10-Mar-27	18
Rayong Lab	Total Dissolved Solids 180°C	Electronic Balance	RYG_EN0163	20-Feb-25	20-Feb-26	12
Rayong Lab	Total Dissolved Solids 180°C	Chamber (Oven)	RYG_EN0012	10-Sep-25	10-Mar-27	18
Rayong Lab	Oil & Grease	Electronic Balance	RYG_EN0003	20-Feb-25	20-Feb-26	12
Rayong Lab	Oil & Grease	Liquid Bath (Water)	RYG_EN0220	27-Nov-25	27-Nov-26	12
Rayong Lab	Color (at Original pH)	Spectrophotometer	RYG_EN0037	18-Mar-25	18-Sep-26	18
Rayong Lab	Color (at pH 7.0)	Spectrophotometer	RYG_EN0037	18-Mar-25	18-Sep-26	18
Rayong Lab	Temperature	pH meter	RYG_FS0605	25-Aug-25	25-Aug-26	12
Rayong Lab	Dissolved Oxygen	Chamber (Cold Room)	RYG_EN0184	27-Nov-25	27-May-27	18
Rayong Lab	COD	Spectrophotometer	RYG_EN0037	18-Mar-25	18-Sep-26	18
Water Lab	n-Hexane	Gas Chromatography (MSD)	BKK_EN0059	25-Jun-25	25-Dec-26	18
Water Lab	TPH C_5-C_8	Gas Chromatography (MSD)	BKK_EN0059	25-Jun-25	25-Dec-26	18
Water Lab	TPH $C_{>8}$-C_{16}	Gas Chromatography (FID)	BKK_EN0411	9-May-25	9-May-26	12
Water Lab	TPH $C_{>16}$-C_{35}	Gas Chromatography (FID)	BKK_EN0411	9-May-25	9-May-26	12
Soil	n-Hexane	Gas Chromatography (MSD)	BKK_EN0059	25-Jun-25	25-Dec-26	18
Soil	pH aqueous phase 50% (w/v)	pH Meter	RYG_EN0152	18-Jun-25	18-Dec-26	18
Soil	TPH C_5-C_8	Gas Chromatography (MSD)	BKK_EN0059	25-Jun-25	25-Dec-26	18
Soil	TPH $C_{>8}$-C_{16}	Gas Chromatography (FID)	BKK_EN0411	9-May-25	9-May-26	12
Soil	TPH $C_{>16}$-C_{35}	Gas Chromatography (FID)	BKK_EN0411	9-May-25	9-May-26	12

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7/139 MOO 13, SOI SUNTINAKORN 11 TAMBON BANG KAEO,
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL.: 0660-2116-5860-1 FAX: 0660-2116-7140

Certificate of Calibration

Customer

Name : ALS Laboratory Group Thailand Co., Ltd.

Address : 104 Soi Phatthanakan 40, Phatthanakan Road, Suan Luang, Bangkok 10250

Certificate No : 25-AFM-023

Request No : Req-2025-0169

Unit Under Calibration Details

Measurement Item : Air Flow Meter

Manufacturer : Mesa Labs — Accuracy : 1% of Reading

Model : 200-510L — Sensor Model : -

Serial Number : 130027 — Sensor Serial Number : -

ID : RYG_FS0208 — Instrument Status : Used

Location of Calibration : LAB 4 AIR VELOCITY METER

Calibration Environment and Details

Temperature : 23 °C ± 3 °C

Humidity : 55 %RH ± 20 %RH

Barometric Pressure : 1013 hPa ± 10 hPa

Received Date : 21 January 2025

Calibration Date : 27 January 2025

Calibration Procedure : In house method CP-AFM-01 by Comparison technique with Standard Primary Flow Calibrator

REVIEW BY .....
APPROVED BY .....
NEXT CAL DATE.....20/01/20.....

Reference Standard	Model	Serial Number	Traceble	Due Calibration
Air Flow Meter	Gilibrator 3 Low flow	18501010006	Sensidyne	6 August 2025
Air Flow Meter	Gilibrator 3 Standard flow	19031011003	Sensidyne	2 August 2025
Temperature meter	GT 11	08000057	Qreborn	1 March 2025
Pressure meter	CPG2400	41000KDU651882	TPA	21 October 2025

Traceability :

This Certificate is traceable to SI Unit through Sensidyne A2LA Accreditation No. 3943.01

Note :

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor $k = 2$, providing a level of confidence approximately 95 %.

Calibration By : Mr. Noppadon Luangart — Service Calibration Engineer

Approved By : Mr. Pacit Mathavorn — Calibration Engineer Supervisor

Issue Date : 27 January 2025

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7/139 MOO 13, SOI SUNTINAKORN 11 TAMBON BANG KAEO,
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL.: 0660-2116-5860-1 FAX: 0660-2116-7140

Certificate No : 25-AFM-023

Request No : Req-2025-0169

Result of Calibration : Without Adjustment

Temperature (°C)	Pressure (kPa)	STD (cc/min)	UUC (cc/min)	Error (cc/min)	Uncertainty (cc/min)	MPE (cc/min)	Result
22.50	100.90	20	19.854	-0.1	1.3	0.2	Pass1
22.50	100.90	50	49.732	-0.3	3.3	0.5	Pass1
22.60	100.90	101	100.77	-0.2	2.8	1.0	Pass1
22.70	100.90	151	150.23	-0.8	4.2	1.5	Pass1
22.70	100.90	201	200.39	-0.6	5.6	2.0	Pass1
22.70	100.90	301	300.69	-0.3	8.4	3.0	Pass1
22.80	100.90	400	402.96	3.0	11	4.0	Pass1
23.10	100.90	500	504.62	4.6	7.2	5.0	Pass1

Note STD : Standard UUC : Unit Under Calibration

- UUC Reference Condition : At atmospheric pressure and room temperature condition
- Flow Rate was corrected for non-standard operating condition by using equation :

$$Q_{meas} = Q_{ref} \, x \, \frac{P_{ref}}{P_{ref}} \, x \, \frac{T_{meas}}{T_{ref}}$$

where Q = Flow Rate P = Absolute Pressure T = Absolute Temperature
Meas = Measurement Condition ref = Standard Condition

* Indicates non accredited

MPE = Maximum Permissible Error (Specified in Manufacturer's Specifications)

N/A = Not Aavailable, Customer does not require a statement of conformity.

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7/139 MOO 13, SOI SUNTINAKORN 11 TAMBON BANG KAEO,
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL.: 0660-2116-5860-1 FAX: 0660-2116-7140

Certificate No : 25-AFM-023

Request No : Req-2025-0169

Decision Rule for Statements of Conformity


The standard decision rule employed for the statements of conformity to each calibration result will be applied using ILAC-G8:09/2019, Guidelines on the Reporting of Compliance with Specification as following Fig. and statements

Pass = The measurement result plus the expanded uncertainty with a 98% coverage probability were within the limit.

Pass[1] = The measurement result was within the limit. However, a portion of the expanded uncertainty of measurement at 95% exceeds the limit.

Fail[1] = The measurement result was out of the limit. However, a portion of the expanded uncertainty of measurement at 95% is within the limit.

Fail = The measurement result plus the expanded uncertainty with a 95% coverage probability were outside the limit.



End of Certificate

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7/139 MOO 13, SOI SUNTINAKORN 11 TAMBON BANG KAEO,
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL.: 0660-2116-5860-1 FAX: 0660-2116-7140

Certificate of Calibration

Customer

Name : ALS Laboratory Group Thailand Co., Ltd.

Address : 104 Soi Phatthanakan 40, Phatthanakan Road, Suan Luang, Bangkok 10250

Certificate No : 24-AFM-179

Request No : Req-2024-1987

Unit Under Calibration Details

Measurement Item : Air Flow Meter

Manufacturer : MesaLabs — Accuracy : 1% of Reading

Model : Defender 510-M — Sensor Model : -

Serial Number : 151114 — Sensor Serial Number : -

ID : BKK_FS0614 — Instrument Status : Used

Location of Calibration : LAB 4 AIR VELOCITY METER

Calibration Environment and Details

Temperature : 23 °C ± 3 °C

Humidity : 55 %RH ± 20 %RH

Barometric Pressure : 1013 hPa ± 10 hPa

Received Date : 30 August 2024

Calibration Date : 9 September 2024

Calibration Procedure : In-house method CP-AFM-01 by Comparison technique with Standard Primary Flow Calibrator

REVIEW BY .....
APPROVED BY .....
NEXT CAL. DATE 9/9/25

Reference Standard	Model	Serial Number	Traceble	Due Calibration
Air Flow Meter	Gilibrator 3 Low flow	18501010006	Sensidyne	6 August 2025
Air Flow Meter	Gilibrator 3 Standard flow	19031011003	Sensidyne	2 August 2025
Temperature meter	GT 11	08000057	Qreborn	1 March 2025
Pressure meter	CPG2400	41000KDU651882	TPA	9 November 2024

Traceability :

This Certificate is traceable to SI Unit through Sensidyne A2LA Accreditation No. 3943.01

Note :

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor $k = 2$, providing a level of confidence approximately 95 %.

Calibration By : Mr. Noppadon Luangart — Service Calibration Engineer

Approved By : Mr. Pacit Mathavorn — Calibration Engineer Supervisor

Issue Date : 9 September 2024

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7/139 MOO 13, SOI SUNTINAKORN 11 TAMBON BANG KAEO,
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL.: 0660-2116-5860-1 FAX: 0660-2116-7140

Certificate No : 24-AFM-179

Request No : Req-2024-1987

Result of Calibration : Without Adjustment

Temperature (°C)	Pressure (kPa)	STD (cc/min)	UUC (cc/min)	Error (cc/min)	Uncertainty (cc/min)	MPE (cc/min)	Result
24.70	100.95	100	100.41	0.4	2.8	1.0	N/A
24.90	100.90	502	500.47	-1.5	7.1	5.0	N/A
24.90	100.97	1003	1001.3	-2	14	10.0	N/A
25.00	100.92	2014	2009.9	-4	29	20.1	N/A
25.20	101.03	3043	3038.3	15	44	30.4	N/A
25.30	101.10	4043	4005.1	-38	57	40.4	N/A
25.50	101.15	5052	5003.9	-48	74	50.5	N/A

Note STD : Standard UUC : Unit Under Calibration

- UUC Reference Condition : At atmospheric pressure and room temperature condition
- Flow Rate was corrected for non-standard operating condition by using equation :

$$Q_{meas} = Q_{ref} \, x \, \frac{P_{ref}}{P_{ref}} \, x \, \frac{T_{meas}}{T_{ref}}$$

where Q = Flow Rate P = Absolute Pressure T = Absolute Temperature
Meas = Measurement Condition ref = Standard Condition

* Indicates non accredited

MPE = Maximum Permissible Error (Specified in Manufacturer's Specifications)

N/A = Not Aavailable, Customer does not require a statement of conformity.

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7/139 MOO 13, SOI SUNTINAKORN 11 TAMBON BANG KAEO,
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL.: 0660-2116-5860-1 FAX: 0660-2116-7140

Certificate No : 24-AFM-179

Request No : Req-2024-1987

Decision Rule for Statements of Conformity


The standard decision rule employed for the statements of conformity to each calibration result will be applied using ILAC-G8:09/2019, Guidelines on the Reporting of Compliance with Specification as following Fig. and statements

Pass = The measurement result plus the expanded uncertainty with a 95% coverage probability were within the limit.

Pass[1] = The measurement result was within the limit. However, a portion of the expanded uncertainty of measurement at 95% exceeds the limit.

Fail[1] = The measurement result was out of the limit. However, a portion of the expanded uncertainty of measurement at 95% is within the limit.

Fail = The measurement result plus the expanded uncertainty with a 95% coverage probability were outside the limit.



End of Certificate

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7/139 MOO 13, SOI SUNTINAKORN 11 TAMBON BANG KAEO,
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL.: 0660-2116-5860-1 FAX: 0660-2116-7140

Certificate of Calibration

Customer

Name : ALS Laboratory Group Thailand Co., Ltd.

Address : 104 Soi Phatthanakan 40, Phatthanakan Road, Suan Luang, Bangkok 10250

Certificate No : 25-AFM-208

Request No : Req-2025-1986

Unit Under Calibration Details

Measurement Item : Air Flow Meter

Manufacturer : Mesa Labs — Sensor Model : -

Model : 200-510M — Sensor Serial Number : -

Serial Number : 151114 — Instrument Status : Used

ID : BKK_FS0614

Location of Calibration : LAB 4 AIR VELOCITY METER

Calibration Environment and Details

Temperature : 23 °C ± 3 °C

Humidity : 55 %RH ± 20 %RH

Barometric Pressure : 1013 hPa ± 10 hPa

Received Date : 3 September 2025

Calibration Date : 10 September 2025

Calibration Procedure : In-house method CP-AFM-01 by Comparison technique with Standard Primary Flow Calibrator

REVIEW BY .....
APPROVED BY .....
NEXT CAL DATE 09/09/26

Reference Standard	Model	serial Number	Traceble	Due Calibration
Air Flow Meter	Gilibrator 3 Low flow	18501010006	Sensidyne	5 May 2026
Air Flow Meter	Gilibrator 3 Standard flow	19031011003	Sensidyne	6 May 2026
Temperature meter	GT 11	08000057	Qreborn	15 October 2025
Pressure meter	CPG2400	41000KDU651882	TPA	21 October 2025

Traceability :

This Certificate is traceable to SI Unit through Sensidyne A2LA Accreditation No. 3943.01 and MIT NSC-TISI-TIS Accreditation No. 0052

Note :

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor $k = 2$, providing a level of confidence approximately 95 %.

Calibration By : Mr. Noppadon Luangart — Service Calibration Engineer

Approved By : Mr. Pacit Mathavorn — Calibration Engineer Supervisor

Issue Date : 10 September 2025

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7/139 MOO 13, SOI SUNTINAKORN 11 TAMBON BANG KAEO,
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL.: 0660-2116-5860-1 FAX: 0660-2116-7140

Certificate No : 25-AFM-208

Request No : Req-2025-1986

Result of Calibration : Without Adjustment

STD Reading			UUC Reading			Error	Uncertainty		
Temperature (°C)	Pressure (kPa)	Flow (cc/min)	Temperature (°C)	Pressure (kPa)	Flow (cc/min)	(cc/min)	(cc/min)	(°C)	(kPa)
25.5	100.98	100	-	-	100.02	0.0	3.6	1.0	0.50
25.7	100.97	503	-	-	500.81	-2.2	9.5	1.0	0.50
25.8	100.89	1003	-	-	1000.4	-3	19	1.0	0.50
26.1	100.88	2000	-	-	2001.9	2	38	1.0	0.50
26.5	100.85	3014	-	-	3002.2	-12	57	1.0	0.50
26.7	100.81	4027	-	-	4000.9	-26	76	1.0	0.50
27.0	100.74	5048	-	-	5001.8	-46	95	1.0	0.50

Note STD : Standard UUC : Unit Under Calibration

- UUC Reference Condition : At atmospheric pressure and room temperature condition, Air
- Flow Rate was corrected for non-standard operating condition by using equation :

$$Qmeas = Qref \, x \, \frac{Pref}{Pmeas} \, x \, \frac{Tmeas}{Tref}$$

where Q = Flow Rate P = Absolute Pressure T = Absolute Temperature
meas = Measurement Condition ref = Standard Condition

* Indicates non accredited

End of Certificate

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7/139 MOO 13, SOI SUNTINAKORN 11 TAMBON BANG KAEO,
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL.: 0660-2116-5860-1 FAX: 0660-2116-7140

Certificate of Calibration

Customer

Name : ALS Laboratory Group Thailand Co., Ltd.

Address : 104 Soi Phatthanakan 40, Phatthanakan Road, Suan Luang, Bangkok 10250

Certificate No : 24-AFM-177

Request No : Req-2024-1862

Unit Under Calibration Details

Measurement Item : Air Flow Meter

Manufacturer : Bios — Accuracy : 1% of Reading

Model : Defender 510-L — Sensor Model : -

Serial Number : 130026 — Sensor Serial Number : -

ID : BKK_FS0619 — Instrument Status : Used

Location of Calibration : LAB 4 AIR VELOCITY METER

Calibration Environment and Details

Temperature : 23 °C ± 3 °C

Humidity : 55 %RH ± 20 %RH

Barometric Pressure : 1013 hPa ± 10 hPa

Received Date : 22 August 2024

Calibration Date : 9 September 2024

Calibration Procedure : In-house method CP-AFM-01 by Comparison technique with Standard Primary Flow Calibrator

REVIEW BY .....
APPROVED BY .....
NEXT CAL. DATE 9/9/26

Reference Standard	Model	Serial Number	Traceble	Due Calibration
Air Flow Meter	Gilibrator 3 Low flow	18501010006	Sensidyne	6 August 2025
Air Flow Meter	Gilibrator 3 Standard flow	19031011003	Sensidyne	2 August 2025
Temperature meter	GT 11	08000057	Qreborn	1 March 2025
Pressure meter	CPG2400	41000KDU651882	TPA	9 November 2024

Traceability :

This Certificate is traceable to SI Unit through Sensidyne A2LA Accreditation No. 3943.01

Note :

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor $k = 2$, providing a level of confidence approximately 95 %.

Calibration By : Mr. Noppadon Luangart — Service Calibration Engineer

Approved By : Mr. Pacit Mathavorn — Calibration Engineer Supervisor

Issue Date : 9 September 2024

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7/139 MOO 13, SOI SUNTINAKORN 11 TAMBON BANG KAEO,
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL: 0669-2116-5869-1 FAX: 0669-2116-7140

Certificate No : 24-AFM-177

Request No : Req-2024-1862

Result of Calibration : Without Adjustment

Temperature (°C)	Pressure (kPa)	STD (cc/min)	UUC (cc/min)	Error (cc/min)	Uncertainty (cc/min)	MPE (cc/min)	Result
24.70	100.92	20	20.192	0.2	1.3	0.2	N/A
24.70	100.99	100	99.923	-0.1	2.8	1.0	N/A
24.70	100.94	201	200.7	-0.3	5.6	2.0	N/A
24.70	100.97	298	300.1	2.1	8.4	3.0	N/A
24.70	100.99	403	399.1	-4	11	4.0	N/A
24.80	101.05	482	477.6	-4.4	6.9	4.8	N/A

Note STD : Standard UUC : Unit Under Calibration

- UUC Reference Condition : At atmospheric pressure and room temperature condition
- Flow Rate was corrected for non-standard operating condition by using equation :

$$Q_{meas} = Q_{ref} \, x \, \frac{P_{ref}}{P_{meas}} \, x \, \frac{T_{meas}}{T_{ref}}$$

where Q = Flow Rate P = Absolute Pressure T = Absolute Temperature
Meas = Measurement Condition ref = Standard Condition

* Indicates non accredited

MPE = Maximum Permissible Error (Specified in Manufacturer's Specifications)

N/A = Not Aavailable, Customer does not require a statement of conformity.

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7/139 MOO 13, SOI SUNTINAKORN 11 TAMBON BANG KAEO,
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL: 0669-2116-5869-1 FAX: 0669-2116-7140

Certificate No : 24-AFM-177

Request No : Req-2024-1862

Decision Rule for Statements of Conformity


The standard decision rule employed for the statements of conformity to each calibration result will be applied using ILAC-G8:09/2019; Guidelines on the Reporting of Compliance with Specification as following Fig. and statements

Pass = The measurement result plus the expanded uncertainty with a 95% coverage probability were within the limit.

Pass' = The measurement result was within the limit. However, a portion of the expanded uncertainty of measurement at 95% exceeds the limit.

Fail' = The measurement result was out of the limit. However, a portion of the expanded uncertainty of measurement at 95% is within the limit.

Fail = The measurement result plus the expanded uncertainty with a 95% coverage probability were outside the limit.



End of Certificate

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

FM-708-AFM-01 Rev.04 Issue date 17/6/24

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7/139 MOO 13, SOI SUNTINAKORN 11 TAMBON BANG KAEO,
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL: 0669-2116-5869-1 FAX: 0669-2116-7140

Certificate of Calibration

Customer

Name : ALS Laboratory Group Thailand Co., Ltd.
Address : 104 Soi Phatthanakan 40, Phatthanakan Road, Suan Luang, Bangkok 10250

Certificate No : 25-AFM-207

Request No : Req-2025-1987

Unit Under Calibration Details

Measurement Item : Air Flow Meter
Manufacturer : Mesa Labs
Model : 200-510L
Serial Number : 130026
ID : BKK_FS0619
Location of Calibration : LAB 4 AIR VELOCITY METER
Sensor Model : -
Sensor Serial Number : -
Instrument Status : Used

Calibration Environment and Details

Temperature : 23 °C ± 3 °C
Humidity : 55 %RH ± 20 %RH
Barometric Pressure : 1013 hPa ± 10 hPa
Received Date : 3 September 2025
Calibration Date : 10 September 2025
Calibration Procedure : In-house method CP-AFM-01 by Comparison technique with Standard Primary Flow Calibrator

REVIEW BY .....
APPROVED BY .....
NEXT CAL DATE.... 09/09/26

Reference Standard	Model	Serial Number	Traceble	Duc Calibration
Air Flow Meter	Gilibrator 3 Low flow	18550130006	Sensidyne	5 May 2026
Air Flow Meter	Gilibrator 3 Standard flow	19031011003	Sensidyne	6 May 2026
Temperature meter	GT 11	68000057	Qualtex	15 October 2025
Pressure meter	CPG2400	410006DR0851882	TPA	21 October 2025

Traceability :
This Certificate is traceable to SI Unit through Sensidyne AZLA Accreditation No. 3943.01 and MIT NSC-TISI-TIS Accreditation No. 0052

Note :
The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor k = 2, providing a level of confidence approximately 95 %.

Calibration By : Mr. Noppadon Luangart, Service Calibration Engineer

Approved By : Mr. Pacit Mathaveen, Calibration Engineer Supervisor

Issue Date : 10 September 2025

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7/139 MOO 13, SOI SUNTINAKORN 11 TAMBON BANG KAEO,
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL: 0669-2116-5869-1 FAX: 0669-2116-7140

Certificate No : 25-AFM-207

Request No : Req-2025-1987

Result of Calibration : Without Adjustment

STD Reading			UUC Reading			Error	Uncertainty		
Temperature (°C)	Pressure (kPa)	Flow (cc/min)	Temperature (°C)	Pressure (kPa)	Flow (cc/min)	(cc/min)	(cc/min)	(°C)	(kPa)
25.5	100.98	20	-	-	20.042	0.0	1.6	1.0	0.50
25.5	100.90	50	-	-	49.921	-0.1	4.0	1.0	0.50
25.5	100.91	100	-	-	100.09	0.1	3.6	1.0	0.50
25.4	100.86	150	-	-	150.34	0.3	5.4	1.0	0.50
25.6	100.93	199	-	-	200.17	1.2	7.2	1.0	0.50
25.6	100.95	301	-	-	300.05	-1	11	1.0	0.50
25.7	100.96	402	-	-	401.03	-1	14	1.0	0.50
25.7	100.95	503	-	-	500.26	-3	10	1.0	0.50

Note STD : Standard UUC : Unit Under Calibration

- UUC Reference Condition : At atmospheric pressure and room temperature condition, Air
- Flow Rate was corrected for non-standard operating condition by using equation :

$$Qmeas = Qref \, x \, \frac{Pref}{Pmeas} \, x \, \frac{Tmeas}{Tref}$$

where Q = Flow Rate P = Absolute Pressure T = Absolute Temperature
meas = Measurement Condition ref = Standard Condition

* Indicates non accredited

End of Certificate

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

FM-708-AFM-01 Rev.06 Issue date 21/3/25

BKK_EN0126

© 2023 by Agilent Technologies Agilent CrossLab Compliance Services

Certificate of System Qualification

GC-OQ

System ID: GC-6_CN11461066
Organization Name: ALS Laboratory Group (Thailand) Co., Ltd.
Organization Location: 104 Soi 40 Phatthanakan Rd,Khwang Suan Luang, Khet Suan Luang, Bangkok 10250

Date: October 22, 2024 9:27:05 AM
EQP Name: AgilentRecommended
EQP Revision: GC.02.53
Overall Qualification Status: Pass

REVIEW BY .....
APPROVED BY .....
NEXT CAL. DATE 22 Apr 2026

CDS Logon Verification - GC

Logon: Saengthai Tarak

Overall CDS Logon Verification - GC Test Status

Pass

System Inspection and Basic Safety and Operation

Name: 7890

Setpoint Status: Pass

Overall System Inspection and Basic Safety and Operation Test Status

Pass

Inlet Pressure Decay

Name: 7890
Front SSL

Setpoint Status: Pass
Pressure: 25.0 psi
Pressure Change: 0.0 psi /5 minutes
Agilent Recommended: >= -2.0 and <= 0.5

© 2023 by Agilent Technologies Agilent CrossLab Compliance Services

Overall Inlet Pressure Decay Test Status

Pass

Inlet Pressure Accuracy

Name: 7890
Front SSL

Setpoint Status: Pass

	Setpoint	Actual	
Inlet Pressure:	25.0 psi	25.07 psi	
Accuracy:		0.1	psi
Agilent Recommended:		<= 1.2	

Overall Inlet Pressure Accuracy Test Status

Pass

Inlet Pressure Decay

Name: 7890
Back SSL

Setpoint Status: Pass
Pressure: 25.0 psi
Pressure Change: 0.0 psi /5 minutes
Agilent Recommended: >= -2.0 and <= 0.5

Overall Inlet Pressure Decay Test Status

Pass

Inlet Pressure Accuracy

Name: 7890
Back SSL

© 2023 by Agilent Technologies Agilent CrossLab Compliance Services

Setpoint Status: Pass

	Setpoint	Actual	
Inlet Pressure:	25.0 psi	25.05 psi	
Accuracy:		0.1	psi
Agilent Recommended:		<= 1.2	

Overall Inlet Pressure Accuracy Test Status

Pass

Detector Flow Accuracy

Name: 7890
Front FID

Setpoint Status: Pass
Flow Type: Fuel
Setpoint: 30.0 mL/min Measured Flow: 28.8 mL/min
Accuracy: 1.2 mL/min
Agilent Recommended: <= 10.0 % setpoint (3.0 ml/min)
Limit is percentage of setpoint or 0.5 ml/minute, whichever is largest.

Setpoint Status: Pass
Flow Type: Oxidizer
Setpoint: 400.0 mL/min Measured Flow: 392 mL/min
Accuracy: 8.0 mL/min
Agilent Recommended: <= 10.0 % setpoint (40.0 ml/min)
Limit is percentage of setpoint or 0.5 ml/minute, whichever is largest.

Setpoint Status: Pass
Flow Type: Makeup
Setpoint: 25.0 mL/min Measured Flow: 25.4 mL/min
Accuracy: 0.4 mL/min
Agilent Recommended: <= 10.0 % setpoint (2.5 ml/min)
Limit is percentage of setpoint or 0.5 ml/minute, whichever is largest.

© 2023 by Agilent Technologies Agilent CrossLab Compliance Services

Overall Detector Flow Accuracy Test Status

Pass

Detector Flow Accuracy

Name: 7890
Back FID

Setpoint Status: Pass
Flow Type: Fuel
Setpoint: 30.0 mL/min Measured Flow: 30.8 mL/min
Accuracy: 0.8 mL/min
Agilent Recommended: <= 10.0 % setpoint (3.0 ml/min)
Limit is percentage of setpoint or 0.5 ml/minute, whichever is largest.

Setpoint Status: Pass
Flow Type: Oxidizer
Setpoint: 400.0 mL/min Measured Flow: 393 mL/min
Accuracy: 7.0 mL/min
Agilent Recommended: <= 10.0 % setpoint (40.0 ml/min)
Limit is percentage of setpoint or 0.5 ml/minute, whichever is largest.

Setpoint Status: Pass
Flow Type: Makeup
Setpoint: 25.0 mL/min Measured Flow: 25.2 mL/min
Accuracy: 0.2 mL/min
Agilent Recommended: <= 10.0 % setpoint (2.5 ml/min)
Limit is percentage of setpoint or 0.5 ml/minute, whichever is largest.

Overall Detector Flow Accuracy Test Status

Pass

GC Oven Temperature Accuracy

Name: 7890

© 2023 by Agilent Technologies Agilent CrossLab Compliance Services

Setpoint Status: Pass
Zone: Oven
Setpoint/Actual

Temperature:	230.0	230.3	°C
Accuracy:		0.3	°C
Agilent Recommended:	>= -1.0	% setpoint in K	(-5.0 °C)
	<= 1.0	% setpoint in K	(5.0 °C)

Setpoint Status: Pass
Zone: Oven
Setpoint/Actual

Temperature:	100.0	100.0	°C
Accuracy:		0.0	°C
Agilent Recommended:	>= -1.0	% setpoint in K	(-3.7 °C)
	<= 1.0	% setpoint in K	(3.7 °C)

Overall GC Oven Temperature Accuracy Test Status

Pass

GC Oven Temperature Stability

Name: 7890

Setpoint Status: Pass
Setpoint/Average

Temperature:	100.0	100.0167	°C
Stability:		0.1	°C
Agilent Recommended:	<=	0.5	

Overall GC Oven Temperature Stability Test Status

Pass

Scouting Run

Tested Combination1 Front SSL / Front FID
Injection Tower
Name: 7693A

Setpoint Status: Completed
Injection Volume on Column: 1.0 uL

Overall Scouting Run Status
Completed

Noise and Drift

Tested Combination1	Front	SSL	/ Front	FID
Name:	7890			

Setpoint Status: Pass
Base Signal: 14.05 pA

	ASTM Noise pA	Drift pA/Hr
	0.05	0.03
Agilent Recommended:	<= 0.10	<= 2.50
Status:	Pass	Pass

Overall Noise and Drift Test Status
Pass

Injection Precision

Tested Combination1	Front:	SSL	/ Front	FID
Name:	7693A			

Setpoint Status: Pass
Injection Volume on Column: 1.0 uL
Area RSD: 0.30 % Retention Time RSD: 0.63 %
Agilent Recommended: <= 3.00 <= 1.00

Overall Injection Precision Test Status
Pass

Signal to Noise

Tested Combination1 Front SSL / Front FID
Injection Tower
Name: 7890

Setpoint Status: Pass
Signal to Noise: 11076525
Agilent Recommended: >= 300000

Overall Signal to Noise Test Status
Pass

Scouting Run

Tested Combination2 Back SSL / Back FID
Injection Tower
Name: 7693A

Setpoint Status: Completed
Injection Volume on Column: 1.0 uL

Overall Scouting Run Status
Completed

Noise and Drift

Tested Combination2 Back SSL / Back FID
Name: 7690

Setpoint Status: Pass
Base Signal: 13.79 pA

	ASTM Noise pA	Drift pA/Hr
	0.05	0.01
Agilent Recommended:	<= 0.10	<= 2.50
Status:	Pass	Pass

Overall Noise and Drift Test Status
Pass

Injection Precision

Tested Combination2 Back SSL / Back FID
Name: 7693A

Setpoint Status: Pass
Injection Volume on Column: 1.0 uL
Area RSD: 1.06 % Retention Time RSD: 0.93 %
Agilent Recommended: <= 3.00 <= 1.00

Overall Injection Precision Test Status
Pass

Signal to Noise

Tested Combination2 Back SSL / Back FID
Injection Tower
Name: 7690

Setpoint Status: Pass
Signal to Noise: 1771221
Agilent Recommended: >= 300000

Overall Signal to Noise Test Status
Pass

Instrument Details

Purpose
This section describes the as found system configuration.

Details

System

System ID	GC-6_CN11461066
Manufacturer	Agilent Technologies
Name	7890
Flow Data Input	Manual Data
Temperature Data Input	Manual Data or Other Data Logging

Tested Combination1

Injection Technique	Injection Tower
Sampler Identifier	Sampler 1
Inlet	Front
Detector	Front
LTM Included?	No

Tested Combination2

Injection Technique	Injection Tower
Sampler Identifier	Sampler 2
Inlet	Back
Detector	Back
LTM Included?	No

Sampler 1

Manufacturer	Agilent Technologies
Type	Injection Tower
Name	7693A
Model Number	G4513A
Serial Number	CNCN10340103
Firmware Revision	A.11.06
Usage	Sample Injection
Location	Front
Syringe Volume (µL)	10

Sampler 2

Manufacturer	Agilent Technologies
Type	Injection Tower
Name	7693A
Model Number	G4513A
Serial Number	CN16280128
Firmware Revision	A.11.06
Usage	Sample Injection
Location	Back
Syringe Volume (µL)	10

Sampler 3

Manufacturer	Agilent Technologies
Type	Tray
Name	7693A
Model Number	G4514A
Serial Number	CN15380030
Firmware Revision	A.11.03
Vial Heater	Not Installed

Mainframe 1

Manufacturer	Agilent Technologies
Name	7890
Model Number	G3440A
Serial Number	CN11461066
Firmware Revision	A.01.16
Oven Type	Standard

Inlet 1

Manufacturer	Agilent Technologies
Name	7890
Type	SSL
Location	Front
Carrier Gas	Helium
Control Type	Electronic Pressure Control (EPC)
Purged Inlet	Yes

Inlet 2

Manufacturer	Agilent Technologies
Name	7890
Type	SSL
Location	Back
Carrier Gas	Helium
Control Type	Electronic Pressure Control (EPC)
Purged Inlet	Yes

Detector 1

Manufacturer	Agilent Technologies
Name	7890
Type	FID
Adapter	Capillary
Control Type	Electronic Pressure Control (EPC)
Location	Front
Makeup Gas	Nitrogen

Detector 2

Manufacturer	Agilent Technologies
Name	7890
Type	FID
Adapter	Capillary
Control Type	Electronic Pressure Control (EPC)
Location	Back
Makeup Gas	Nitrogen

Electronic Signature

Purpose
This signature page was created and published because the ACE sign-off action was executed, which is valid for the entire document, including attachments. The ACE sign-off is an electronic signature that requires two distinct identification components: unique username and personal password. The Agilent representative who has delivered this service understands the meaning and legal status of an electronic signature. As a trained official operator, the Agilent representative has a unique password and logon to access ACE and electronically sign this document. (Other e-signatures can be applied to this document using a Document Content Management or other suitable method defined in your data access and control procedures.)

Details

Full Name of Signer:	Saengulthai Terak
Logged On User Name:	saengulthai.terak@hor.agilent.com
Signature Creation Date:	October 22, 2024
Reason for Signature:	Executed protocol and published this original version of document

Regulatory Disclaimer

This document provides a protocol to verify and record instrument configuration and evidence of proper operation. It has been prepared from our interpretation of applicable regulations as well as industry best practices. The document is designed to provide an important component of a complete compliance package. Validation depends upon many factors and use of this protocol alone does not assure compliance. Agilent Technologies makes no promises or representations as to its sufficiency for any specific regulatory program.

Warranty

Agilent Technologies makes no warranty of any kind to this material, including but not limited to, the implied warranties or merchantability and fitness for a particular purpose. Agilent Technologies shall not be liable for errors contained herein or for incidental or consequential damages in connection with the furnishing, performance, or use of this material.

User Name: saengulthai.terak
Report Generated by Hostname: LAPTOP-CO3SKOMV
System Id: GC-6_CN11461066
Print Date: October 22, 2024 9:27:06 AM

2024_ALS_GC-6_CN11461066_OQIHW Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
October 21, 2024 3:16:06 PM	Audit	SessionCreated	Session	None
October 21, 2024 3:16:07 PM	Start	Configuration	Session	None
October 21, 2024 3:16:07 PM	Audit	fmMement	Licensing	User is nonpaying and does not require an unlock code
October 21, 2024 3:22:10 PM	Audit	ProjLoaded	Session	EDP details for primary technique [Sq] - File path: [ProtocolPacks/GcConfigurations/GC SQ/GC SQ.S2q]. EDP File Name: [Gc.02.53.sqg], EDP Name: [AgilentRecommended],Protocol Revision [Gc.02.53]
October 21, 2024 3:22:44 PM	End	Configuration	Session	None
October 21, 2024 3:22:47 PM	Start	Qualification	Session	OQ
October 21, 2024 3:23:48 PM	Start	Execution	CDS Logon Verification - GC - 7890. - Qualitative test	None
October 21, 2024 3:23:58 PM	End	Execution	CDS Logon Verification - GC - 7890. - Qualitative test	Run Count: 1
October 21, 2024 3:23:45 PM	Start	Execution	System Inspection and Basic Safety and Operation - 7890: - Qualitative Test - No setpoints associated	None
October 21, 2024 3:23:59 PM	End	Execution	System Inspection and Basic Safety and Operation - 7890: - Qualitative Test - No setpoints associated	Run Count: 1

User Name: saengulthai.terak
Report Generated by Hostname: LAPTOP-CO3SKOMV
System Id: GC-6_CN11461066
Print Date: October 22, 2024 9:27:06 AM

2024_ALS_GC-6_CN11461066_OQIHW Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
October 21, 2024 3:24:01 PM	Start	Execution	Inlet Pressure Decay - Front SSL: - Pressure Controlled Inlet - S: 25.0 psi - L: >= -2.0 psi and <= 0.5 psi	None
October 21, 2024 3:25:06 PM	End	Execution	Inlet Pressure Decay - Front SSL: - Pressure Controlled Inlet - S: 25.0 psi - L: >= -2.0 psi and <= 0.5 psi	Run Count: 1
October 21, 2024 3:26:26 PM	Start	Execution	Inlet Pressure Accuracy - Front SSL: - Pressure Controlled Inlet - S: 25.0 psi - L: <= 1.2 psi	None
October 21, 2024 3:26:32 PM	End	Execution	Inlet Pressure Accuracy - Front SSL: - Pressure Controlled Inlet - S: 25.0 psi - L: <= 1.2 psi	Run Count: 1
October 21, 2024 3:25:50 PM	Start	Execution	Inlet Pressure Decay - Back SSL: - Pressure Controlled Inlet - S: 25.0 psi - L: >= -2.0 psi and <= 0.5 psi	None
October 21, 2024 3:26:01 PM	End	Execution	Inlet Pressure Decay - Back SSL: - Pressure Controlled Inlet - S: 25.0 psi - L: >= -2.0 psi and <= 0.5 psi	Run Count: 1
October 21, 2024 3:26:05 PM	Start	Execution	Inlet Pressure Accuracy - Back SSL: - Pressure Controlled Inlet - S: 25.0 psi - L: <= 1.2 psi	None
October 21, 2024 3:26:10 PM	End	Execution	Inlet Pressure Accuracy - Back SSL: - Pressure Controlled Inlet - S: 25.0 psi - L: <= 1.2 psi	Run Count: 1
October 21, 2024 3:26:12 PM	Start	Execution	Detector Flow Accuracy - Front FID: - Type: - Front - S: 30.0 mL/min - L: <= 10.0% setpoint	None

© 2023 by Agilent Technologies

User Name: saengsithal.tarok
Report Generated by Hostname: LAPTOP-CQ35KOMV
System Id: GC-6_CN11461066
Print Date: October 22, 2024 9:27:06 AM

2024_ALS_GC-6_CN11461066_OQHW Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
October 21, 2024 3:29:00 PM	Audit	Data	Detector Flow Accuracy - Front FID - Type : Fuel - S: 30.0 mL/min - L: <= 10.0% setpoint	Manual Data Entry
October 21, 2024 3:29:53 PM	End	Execution	Detector Flow Accuracy - Front FID - Type : Fuel - S: 30.0 mL/min - L: <= 10.0% setpoint	Run Count : 1
October 21, 2024 3:30:54 PM	Start	Execution	Detector Flow Accuracy - Front FID - Type : Oxidizer - S: 400.0 mL/min - L: <= 10.0% setpoint	None
October 21, 2024 3:31:53 PM	Audit	Data	Detector Flow Accuracy - Front FID - Type : Oxidizer - S: 400.0 mL/min - L: <= 10.0% setpoint	Manual Data Entry
October 21, 2024 3:32:53 PM	End	Execution	Detector Flow Accuracy - Front FID - Type : Oxidizer - S: 400.0 mL/min - L: <= 10.0% setpoint	Run Count : 1
October 21, 2024 3:33:54 PM	Start	Execution	Detector Flow Accuracy - Front FID - Type : Makeup - S: 25.0 mL/min - L: <= 10.0% setpoint	None
October 21, 2024 3:34:53 PM	Audit	Data	Detector Flow Accuracy - Front FID - Type : Makeup - S: 25.0 mL/min - L: <= 10.0% setpoint	Manual Data Entry
October 21, 2024 3:35:53 PM	End	Execution	Detector Flow Accuracy - Front FID - Type : Makeup - S: 25.0 mL/min - L: <= 10.0% setpoint	Run Count : 1
October 21, 2024 3:36:54 PM	Start	Execution	Detector Flow Accuracy - Back FID - Type : Fuel - S: 30.0 mL/min - L: <= 10.0% setpoint	None
October 21, 2024 3:37:53 PM	Audit	Data	Detector Flow Accuracy - Back FID - Type : Fuel - S: 30.0 mL/min - L: <= 10.0% setpoint	Manual Data Entry
October 21, 2024 3:37:53 PM	End	Execution	Detector Flow Accuracy - Back FID - Type : Fuel - S: 30.0 mL/min - L: <= 10.0% setpoint	Run Count : 1

Date: October 22, 2024 9:27:05 AM
System ID: GC-6_CN11461066

© 2023 by Agilent Technologies

User Name: saengsithal.tarok
Report Generated by Hostname: LAPTOP-CQ35KOMV
System Id: GC-6_CN11461066
Print Date: October 22, 2024 9:27:05 AM

2024_ALS_GC-6_CN11461066_OQHW Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
October 21, 2024 3:29:54 PM	Start	Execution	Detector Flow Accuracy - Back FID - Type : Oxidizer - S: 400.0 mL/min - L: <= 10.0% setpoint	None
October 21, 2024 3:30:37 PM	Audit	Data	Detector Flow Accuracy - Back FID - Type : Oxidizer - S: 400.0 mL/min - L: <= 10.0% setpoint	Manual Data Entry
October 21, 2024 3:30:09 PM	End	Execution	Detector Flow Accuracy - Back FID - Type : Oxidizer - S: 400.0 mL/min - L: <= 10.0% setpoint	Run Count : 1
October 21, 2024 3:30:11 PM	Start	Execution	Detector Flow Accuracy - Back FID - Type : Makeup - S: 25.0 mL/min - L: <= 10.0% setpoint	None
October 21, 2024 3:30:34 PM	Audit	Data	Detector Flow Accuracy - Back FID - Type : Makeup - S: 25.0 mL/min - L: <= 10.0% setpoint	Manual Data Entry
October 21, 2024 3:30:37 PM	End	Execution	Detector Flow Accuracy - Back FID - Type : Makeup - S: 25.0 mL/min - L: <= 10.0% setpoint	Run Count : 1
October 21, 2024 3:30:38 PM	Start	Execution	GC Oven Temperature Accuracy - 7090 - Temperature : Oven - S: 230.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	None
October 21, 2024 3:31:56 PM	Audit	Data	GC Oven Temperature Accuracy - 7090 - Temperature : Oven - S: 230.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	Manual Data Entry
October 21, 2024 3:31:57 PM	End	Execution	GC Oven Temperature Accuracy - 7890 - Temperature : Oven - S: 230.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	Run Count : 1

Date: October 22, 2024 9:27:05 AM
System ID: GC-6_CN11461066

© 2023 by Agilent Technologies

User Name: saengsithal.tarok
Report Generated by Hostname: LAPTOP-CQ35KOMV
System Id: GC-6_CN11461066
Print Date: October 22, 2024 9:27:05 AM

2024_ALS_GC-6_CN11461066_OQHW Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
October 21, 2024 3:31:53 PM	Start	Execution	GC Oven Temperature Accuracy - 7890 - Temperature : Oven - S: 100.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	None
October 21, 2024 3:34:37 PM	Audit	Data	GC Oven Temperature Accuracy - 7890 - Temperature : Oven - S: 100.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	Manual Data Entry
October 21, 2024 3:34:39 PM	End	Execution	GC Oven Temperature Accuracy - 7890 - Temperature : Oven - S: 100.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	Run Count : 1
October 21, 2024 3:34:42 PM	Start	Execution	GC Oven Temperature Stability - 7890 - Temperature : Oven - S: 100.0°C - L: <= 0.5°C	None
October 21, 2024 3:35:05 PM	Audit	Data	GC Oven Temperature Stability - 7890 - Temperature : Oven - S: 100.0°C - L: <= 0.5°C	Manual Data Entry
October 21, 2024 3:36:07 PM	End	Execution	GC Oven Temperature Stability - 7890 - Temperature : Oven - S: 100.0°C - L: <= 0.5°C	Run Count : 1
October 21, 2024 3:59:33 PM	Start	Execution	GC Scouting Run - Injection Tower, Front SSL, Front FID: - Part of System Preparation - No limits associated	None
October 21, 2024 3:49:12 PM	Audit	AceClosed	Session	None
October 22, 2024 8:55:47 AM	Audit	AceRestarted	Session	None
October 22, 2024 8:55:50 AM	Audit	SessionReloaded	Session	None
October 22, 2024 8:56:02 AM	Start	Qualification	Session	OQ

Date: October 22, 2024 9:27:05 AM
System ID: GC-6_CN11461066

© 2023 by Agilent Technologies

User Name: saengsithal.tarok
Report Generated by Hostname: LAPTOP-CQ35KOMV
System Id: GC-6_CN11461066
Print Date: October 22, 2024 9:27:06 AM

2024_ALS_GC-6_CN11461066_OQHW Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
October 22, 2024 8:58:02 AM	Start	Execution	GC Scouting Run - Injection Tower, Front SSL, Front FID: - Part of System Preparation - No limits associated	None
October 22, 2024 8:58:46 AM	Audit	Data	GC Scouting Run - Injection Tower, Front SSL, Front FID: - Part of System Preparation - No limits associated	Data files Path : G:\Data\Front\Front_SC10.D\ FID1A.ch
October 22, 2024 8:57:25 AM	End	Execution	GC Scouting Run - Injection Tower, Front SSL, Front FID: - Part of System Preparation - No limits associated	Run Count : 1
October 22, 2024 8:57:59 AM	Start	Execution	Noise and Drift - Front FID: - Detector FID - L (Noise): <= 0.10 pA - L (Drift): <= 2.50 pA/hour	None
October 22, 2024 8:58:37 AM	End	Execution	Noise and Drift - Front FID: - Detector FID - L (Noise): <= 0.10 pA - L (Drift): <= 2.50 pA/hour	Run Count : 1
October 22, 2024 8:58:40 AM	Start	Execution	Injection Precision - Injection Tower, Front SSL, Front FID: - GC - L (Area): <= 3.00% - L (Ret. Time): <= 1.00%	None
October 22, 2024 8:59:00 AM	Audit	Data	DataManager	DataManager was in a data verification state but the user chose to start over

Date: October 22, 2024 9:27:05 AM
System ID: GC-6_CN11461066

© 2023 by Agilent Technologies

User Name: saengsithal.tarok
Report Generated by Hostname: LAPTOP-CQ35KOMV
System Id: GC-6_CN11461066
Print Date: October 22, 2024 9:27:06 AM

2024_ALS_GC-6_CN11461066_OQHW Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
October 22, 2024 9:01:43 AM	Audit	Data	Injection Precision - Injection Tower, Front SSL, Front FID: - GC - L (Area): <= 3.00% - L (Ret. Time): <= 1.00%	Data files Path : G:\Data\Front\Front_IP0105.D\ FID1A.ch
October 22, 2024 9:01:43 AM	Audit	Data	Injection Precision - Injection Tower, Front SSL, Front FID: - GC - L (Area): <= 3.00% - L (Ret. Time): <= 1.00%	Data files Path : G:\Data\Front\Front_IP0106.D\ FID1A.ch
October 22, 2024 9:01:43 AM	Audit	Data	Injection Precision - Injection Tower, Front SSL, Front FID: - GC - L (Area): <= 3.00% - L (Ret. Time): <= 1.00%	Data files Path : G:\Data\Front\Front_IP0107.D\ FID1A.ch
October 22, 2024 9:01:43 AM	Audit	Data	Injection Precision - Injection Tower, Front SSL, Front FID: - GC - L (Area): <= 3.00% - L (Ret. Time): <= 1.00%	Data files Path : G:\Data\Front\Front_IP0108.D\ FID1A.ch
October 22, 2024 9:01:43 AM	Audit	Data	Injection Precision - Injection Tower, Front SSL, Front FID: - GC - L (Area): <= 3.00% - L (Ret. Time): <= 1.00%	Data files Path : G:\Data\Front\Front_IP0109.D\ FID1A.ch
October 22, 2024 9:01:43 AM	Audit	Data	Injection Precision - Injection Tower, Front SSL, Front FID: - GC - L (Area): <= 3.00% - L (Ret. Time): <= 1.00%	Data files Path : G:\Data\Front\Front_IP0110.D\ FID1A.ch
October 22, 2024 9:02:11 AM	End	Execution	Injection Precision - Injection Tower, Front SSL, Front FID: - GC - L (Area): <= 3.00% - L (Ret. Time): <= 1.00%	Run Count : 1
October 22, 2024 9:02:16 AM	Start	Execution	Signal to Noise - Injection Tower, Front SSL, Front FID: - Detector FID - L: >= 300000	None
October 22, 2024 9:02:24 AM	Audit	Data	Signal to Noise - Injection Tower, Front SSL, Front FID: - Detector FID - L: >= 300000	Data files Path : G:\Data\Front\Front_SN01.D\ FID1A.ch

Date: October 22, 2024 9:27:05 AM
System ID: GC-6_CN11461066

© 2023 by Agilent Technologies

User Name: saengsithal.tarok
Report Generated by Hostname: LAPTOP-CQ35KOMV
System Id: GC-6_CN11461066
Print Date: October 22, 2024 9:27:06 AM

2024_ALS_GC-6_CN11461066_OQHW Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
October 22, 2024 9:62:04 AM	End	Execution	Signal to Noise - Injection Tower, Front SSL, Front FID: - Detector FID - L: >= 300000	Run Count : 1
October 22, 2024 9:03:00 AM	Start	Execution	GC Scouting Run - Injection Tower, Back SSL, Back FID: - Part of System Preparation - No limits associated	None
October 22, 2024 9:03:31 AM	Audit	Data	GC Scouting Run - Injection Tower, Back SSL, Back FID: - Part of System Preparation - No limits associated	Data files Path : G:\Data\Back\Back_SC01.D\ FID2B.ch
October 22, 2024 9:04:03 AM	End	Execution	GC Scouting Run - Injection Tower, Back SSL, Back FID: - Part of System Preparation - No limits associated	Run Count : 1
October 22, 2024 9:04:06 AM	Start	Execution	Noise and Drift - Back FID: - Detector FID - L (Noise): <= 0.10 pA - L (Drift): <= 2.50 pA/hour	None
October 22, 2024 9:08:56 AM	Audit	Data	Noise and Drift - Back FID: - Detector FID - L (Noise): <= 0.10 pA - L (Drift): <= 2.50 pA/hour	Data files Path : G:\Data\Back\Back_ND013.D\ FID2B.ch
October 22, 2024 9:09:13 AM	End	Execution	Noise and Drift - Back FID: - Detector FID - L (Noise): <= 0.10 pA - L (Drift): <= 2.50 pA/hour	Run Count : 1
October 22, 2024 9:09:16 AM	Start	Execution	Injection Precision - Injection Tower, Back SSL, Back FID: - GC - L (Area): <= 3.00% - L (Ret. Time): <= 1.00%	None

Date: October 22, 2024 9:27:05 AM
System ID: GC-6_CN11461066

© 2023 by Agilent Technologies

User Name: saengsithal.tarok
Report Generated by Hostname: LAPTOP-CQ35KOMV
System Id: GC-6_CN11461066
Print Date: October 22, 2024 9:27:06 AM

2024_ALS_GC-6_CN11461066_OQHW Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
October 22, 2024 9:10:04 AM	Audit	Data	Injection Precision - Injection Tower, Back SSL, Back FID: - GC - L (Area): <= 3.00% - L (Ret. Time): <= 1.00%	Data files Path : G:\Data\Back\Back_IP0111.D\ FID2B.ch
October 22, 2024 9:10:44 AM	Audit	Data	Injection Precision - Injection Tower, Back SSL, Back FID: - GC - L (Area): <= 3.00% - L (Ret. Time): <= 1.00%	Data files Path : G:\Data\Back\Back_IP0112.D\ FID2B.ch
October 22, 2024 9:10:41 AM	Audit	Data	Injection Precision - Injection Tower, Back SSL, Back FID: - GC - L (Area): <= 3.00% - L (Ret. Time): <= 1.00%	Data files Path : G:\Data\Back\Back_IP0113.D\ FID2B.ch
October 22, 2024 9:10:44 AM	Audit	Data	Injection Precision - Injection Tower, Back SSL, Back FID: - GC - L (Area): <= 3.00% - L (Ret. Time): <= 1.00%	Data files Path : G:\Data\Back\Back_IP0114.D\ FID2B.ch
October 22, 2024 9:10:44 AM	Audit	Data	Injection Precision - Injection Tower, Back SSL, Back FID: - GC - L (Area): <= 3.00% - L (Ret. Time): <= 1.00%	Data files Path : G:\Data\Back\Back_IP0115.D\ FID2B.ch
October 22, 2024 9:10:44 AM	Audit	Data	Injection Precision - Injection Tower, Back SSL, Back FID: - GC - L (Area): <= 3.00% - L (Ret. Time): <= 1.00%	Data files Path : G:\Data\Back\Back_IP0116.D\ FID2B.ch
October 22, 2024 9:11:15 AM	End	Execution	Injection Precision - Injection Tower, Back SSL, Back FID: - GC - L (Area): <= 3.00% - L (Ret. Time): <= 1.00%	Run Count : 1
October 22, 2024 9:11:23 AM	Start	Execution	Signal to Noise - Injection Tower, Back SSL, Back FID: - Detector FID - L: >= 300000	None
October 22, 2024 9:11:45 AM	Audit	Data	Signal to Noise - Injection Tower, Back SSL, Back FID: - Detector FID - L: >= 300000	Data files Path : G:\Data\Back\Back_SN01.D\ FID2B.ch

Date: October 22, 2024 9:27:05 AM
System ID: GC-6_CN11461066

© 2023 by Agilent Technologies

User Name: saengsithal.tarok
Report Generated by Hostname: LAPTOP-CQ35KOMV
System Id: GC-6_CN11461066
Print Date: October 22, 2024 9:27:06 AM

2024_ALS_GC-6_CN11461066_OQHW Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
October 22, 2024 9:12:08 AM	End	Execution	Signal to Noise - Injection Tower, Back SSL, Back FID: - Detector FID - L: >= 300000	Run Count : 1
October 22, 2024 9:12:15 AM	End	Qualification	Session	OQ
October 22, 2024 9:12:15 AM	Start	Reporting	Session	None
October 22, 2024 9:24:05 AM	Audit	Reporting	Session	Report Generated : Certificate
October 22, 2024 9:25:56 AM	Audit	Reporting	Session	Report Generated : Report

Date: October 22, 2024 9:27:05 AM
System ID: GC-6_CN11461066

© 2023 by Agilent Technologies

User Name: saengsithal.tarok
Report Generated by Hostname: LAPTOP-CQ35KOMV
System Id: GC-6_CN11461066
Print Date: October 22, 2024 9:27:06 AM

2024_ALS_GC-6_CN11461066_OQHW Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
October 22, 2024 9:12:08 AM	End	Execution	Signal to Noise - Injection Tower, Back SSL, Back FID: - Detector FID - L: >= 300000	Run Count : 1
October 22, 2024 9:12:15 AM	End	Qualification	Session	OQ
October 22, 2024 9:12:15 AM	Start	Reporting	Session	None
October 22, 2024 9:24:05 AM	Audit	Reporting	Session	Report Generated : Certificate
October 22, 2024 9:25:56 AM	Audit	Reporting	Session	Report Generated : Report

Date: October 22, 2024 9:27:05 AM
System ID: GC-6_CN11461066

JNAC
JIRANATEE ASSOCIATES CO.,LTD.
Jiranatee Associates Co.,Ltd
63/34-35, 63/35-36
Petchkasem 7,7/1, Rd. Nakhonpatha, Bangkoyai,
Bangkok 10600,Thailand
Tel: +6629889812
Mobile: +66819319453
E-mail: jnac-calibration@jiranatee.com
Web site: www.jiranatee.com

Accredited calibration laboratory
ISO/IEC 17025:2017
NSC TIS 17025
CALIBRATION 0367

Air speed measurement laboratory
Calibration services department.

ilac-MRA
NSC – TISI – TIS 17025
CALIBRATION 0367

Certificate Number
CWS-013-68

CERTIFICATE OF CALIBRATION

Page 1 of 2 Pages

MEASUREMENT ITEM	: Cup anemometer	
MANUFACTURER	: Novalynx	
MODEL/TYPE	: Sensor: WS-D2#	
	Data logger: 200-WS-2S1B	
SERIAL NUMBER	: Sensor: WSD-A5190	
	Data logger: A5190	
ID NUMBER	: RYG_FS0329	
CONDITION AS-RECEIVED	: Used item	
CUSTOMER	: AIS laboratory group (Thailand) Co, Ltd. 104 Phatthanakan 40, Phatthanakan Rd, Khwaeng Suan Luang, Khet Suan Luang, Bangkok 10250 Thailand.	
RECEIVED DATE	: 18 Apr 2025	
MEASUREMENT DATE	: 07 May 2025	
ISSUE DATE	: 09 May 2025	
ENVIRONMENTAL CONDITIONS:		
Ambient condition in the laboratory are as follow:		
Temperature	: 23.0 ± 3.0	°C
Relative Humidity	: 55.0 ± 15.0	%RH
Atmospheric Pressure	: 1018± 10	hPa
PLACE OF CALIBRATION	: Effel-type wind tunnel of Jiranatee Associates Co., Ltd.	
CALIBRATION CONDITIONS	: Wind tunnel cross-section area	900 cm²
	Cup anemometer frontal area	102 cm²
	Diameter of mounting pipe	- mm
	Blockage ratio of test object*	0.111 [-]
Preconditioning	: 24 hours at ambient conditions.	
Measurement Condition	: The average values during measurement are (24.3) °C, (41.2) %RH and (1008.7) hPa.	

Calibration procedure:
The Cup anemometer was calibrated against Standard air velocity transducer model: 8455IQ2 and pitot tube with precision differential pressure meter model: DPM1500 in an open test section of Effel-type wind tunnel with 900 cm² cross test section area. The WI-CL-002 based on IEC 61400-12-1, Wind energy generation systems – Part 12-1: Power performance measurements of electricity producing wind turbines, March 2017 was used as a calibration guideline.

Traceability:
This certificate provides a traceability of the measurement to recognized the national standards, and to realization of the international system of units (SI) through the NIMT (National Metrology Institute of Thailand) via Certificate number: MW-0019-25 and MW-0055-24.

Uncertainty of Measurement:
The reported uncertainty of measurement is based on the standard uncertainty multiplied by a coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty has been determined in accordance with the GUM "Evaluation of measurement data – Guide to the expression of uncertainty in measurement"

TABULATION OF RESULTS:
The table on next page give the measured values.

Calibrated by:
☐ Mr. Sorawit Thaopiboon
☒ Miss. Wirayanee Lertsongkhod

Approved signatory: .....
Mr. Parinya Boonchuensri
Calibration Department Manager

REVIEW BY .....
APPROVED BY .....
NEXT CAL DATE 06 / 11 /2026

Remarks:
* Normal to the section area of the wind tunnel
Projected cross-section area of the tested object include mounting pipe
Diameter of mounting pipe
Ratio "a"

THIS CERTIFICATE OF CALIBRATION MAY NOT BE REPRODUCED EXCEPT IN FULL UNLESS PERMISSION FOR REPRODUCTION HAS BEEN OBTAINED IN WRITING FROM THE LABORATORY

Jiranatee Associates

Certificate Number
CWS-013-68

MEASUREMENT RESULTS [1]

The Cup anemometer, Unit Under Calibration (UUC) was exercise at 10 m/s for 5minutes prior to calibration being performed. The standard air velocity 0.5 m/s to 5 m/s was calculated by a standard air velocity transducer which was installed 50 mm away from wind tunnel nozzle and installed 40 mm away from top of the test section and the standard air velocity 5 m/s to 30 m/s was calculated by a pitot tube with precision differential pressure meter which was installed 50 mm away from wind tunnel nozzle and installed 40 mm away from top of the test section, UUC was mounted on a round vertical tube at the lower plate at center of test section. The calibration was carried out under both rising and falling air velocity in the range of 1 m/s to 16 m/s at calibration interval of 1 m/s. The results of calibration and associated measurement uncertainties are reported in the table below.

V_{ref} [2] (m/s)	Temp. wind tunnel (°C)	Temp. room (°C)	V_{unc} [3] (m/s)	Error (m/s)	U (k=2) (m/s)
1.018	24.30	24.30	0.8	-0.2	0.31
2.113	24.70	24.30	2.0	-0.3	0.31
3.060	24.50	24.30	3.0	-0.1	0.31
4.378	24.46	24.30	4.0	-0.3	0.31
4.95	24.66	24.30	5.0	0.1	0.31
5.96	24.56	24.30	6.1	0.1	0.31
7.03	24.50	24.30	7.1	0.1	0.31
7.96	24.62	24.30	8.1	0.2	0.31
9.04	24.52	24.30	9.2	0.2	0.31
10.00	24.38	24.30	10.2	0.2	0.31
10.98	24.50	24.30	11.1	0.2	0.31
11.98	24.20	24.30	12.3	0.3	0.31
12.97	24.58	24.30	13.3	0.3	0.31
14.00	24.30	24.30	14.3	0.3	0.34
14.99	24.50	24.30	15.3	0.3	0.31
15.99	24.38	24.30	16.4	0.4	0.35

Remark:

[1] Calibration results only count for the tested circumstances and environmental conditions during which calibration took place

[2] Velocity of standard

[3] Velocity of Unit Under Calibration

PHOTO OF CALIBRATION SET-UP



Calibration set-up of the Cup anemometer calibration in the wind tunnel of Jiranatee Associates Co., Ltd. The Cup anemometer shown may differ from the calibrated one. Remark: The proportion of the set- up is not true to scale due to imaging geometry.

End of Certificate of Calibration

JIRANATEE ASSOCIATES CO.,LTD.

Jiranatee Associates Co., Ltd.

JIRANATEE ASSOCIATES CO.,LTD.

Jiranatee Associates Co.,Ltd
63/14-15, 67/35-36
Petchkasem 7,7/1, Rd. Watthaya, Bangkokyai,
Bangkok 10600(Thailand)
Tel: +66(0)868308312
Mobile: +66(0)899599453
E-mail: jnac-calibration@jiranatee.com
Web site: www.jiranatee.com

Accredited calibration laboratory
ISO/IEC 17025:2017
NSC-TISI-TIS 17025
CALIBRATION 0367

Wind direction measurement laboratory
Calibration services department.

NSC – TISI – TIS 17025
CALIBRATION 0367

Certificate Number
CW3-013-68

CERTIFICATE OF CALIBRATION

MEASUREMENT ITEM	: Wind Direction Sensor		
MANUFACTURER	: Novalynx		
MODEL/TYPE	: Sensor: WS-02F Data logger: 200-WS-25LB		
SERIAL NUMBER	: Sensor: WSD-A5190 Data logger: A5190		
ID NUMBER	: RYG_FS0329		
CONDITION AS-RECEIVED	: Used item		
CUSTOMER	: ALS laboratory group (Thailand) Co., ltd. 104 Phatthanakan 40, Phatthanakan Rd, Khwaeng Suan Luang, Khet Suan Luang, Bangkok 10250 Thailand.		
RECEIVED DATE	: 18 Apr 2025		
MEASUREMENT DATE	: 07 May 2025		
ISSUE DATE	: 09 May 2025		
ENVIRONMENTAL CONDITIONS:			
Ambient condition in the laboratory are as follow:			
Temperature	: 23.0 ± 3.0	°C	
Relative Humidity	: 55.0 ± 15.0	%RH	
Atmospheric Pressure	: 1010 ± 10	hPa	
PLACE OF CALIBRATION	: Eiffel-type wind tunnel of Jiranatee Associates Co., Ltd.		
CALIBRATION CONDITION	: Wind tunnel cross-section area[1]	900	cm^2
	Wind direction frontal area[2]	129	cm^2
	Diameter of mounting pipe[3]	-	mm
	Blockage ratio of test object[4]	0.143	[-]
Preconditioning	: 24 hours at ambient conditions.		
Measurement Condition	: The average values during measurement are (24.4)°C, (43.6) %RH and (1010.9) hPa.		

Calibration procedure:

The wind direction sensor was calibrated against Standard Rotary Encoder, model: AX4003T5-DMX4-P3-S-00 in an close test-section of Eiffel-type wind tunnel with 900 cm^2 cross test section area. The WI-CL-008 based on IEC 61400-12-1, Wind energy generation systems – Part 12-1: Power performance measurements of electricity producing wind turbines, March 2017 was used as a calibration guideline.

Traceability:

This certificate provides a traceability of The measurement to recognized the national standards, and to realization of the international system of units (SI) through the NIMT (National Metrology Institute of Thailand) via Certificate number: 04-0027-24.

Uncertainty of Measurement:

The reported uncertainty of measurement is based on the standard uncertainty multiplied by a coverage factor k=2, Which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty has been determined in accordance with the GUM 'Evaluation of measurement data - Guide to the expression of uncertainty in measurement'

TABULATION OF RESULTS:

The table on next page give the measured values.

Calibrated by:

☐ Mr. Sorawit Thachalad

☑ Miss Jittraporn Lertsomphol

Approved signatory: .....

Mr. Parinya Booncharoen
Calibration Department Manager

Remark:

[1] Nozzle cross-section area of the wind tunnel

[2] Projected cross-section area of the tested object include mounting pipe

[3] Diameter of mounting pipe

[4] Ratio [2] to [1]

THIS CERTIFICATE OF CALIBRATION MAY NOT BE REPRODUCED EXCEPT IN FULL UNLESS PERMISSION FOR REPRODUCTION HAS BEEN OBTAINED IN WRITING FROM THE LABORATORY

Certificate Number
CWD-013-68

MEASUREMENT RESULTS [1]

The wind direction sensor was calibrated against standard rotary encoder by comparison method. During calibration, the measurement was carried out at 45° intervals in clockwise and counterclockwise directions after offset adjustment has been made. The flow speed of wind tunnel (usually 5 m/s) is kept constant while the sensor is rotated around its vertical axis. The results of calibration and associated measurement uncertainties are reported in the table below.

Air speed m/s	θ'_{ref} Degree (°)	θ'_{unc} Degree (°)	Error Degree (°)	U (k=2) Degree (°)
5.01	45.000	41	-4	0.80
	90.000	87	-3	0.80
	135.000	132	-3	0.80
	180.001	178	-2	0.80
	225.000	226	1	0.80
	270.000	273	3	0.80
	315.000	320	5	0.80
	360.000	359	-1	0.80

Remark:

[1] Calibration results only count for the tested circumstances and environmental conditions during which calibration took place

[2] Direction of standard

[3] Direction of Unit Under Calibration

End of Certificate of Calibration

JIRANATEE ASSOCIATES CO.,LTD.

Jiranatee Associates Co., Ltd.

JIRANATEE ASSOCIATES CO.,LTD.

Jiranatee Associates Co.,Ltd
63/14-15, 67/35-36
Petchkasem 7,7/1, Rd. Watthaya, Bangkokyai,
Bangkok 10600(Thailand)
Tel: +66(0)868308312
Mobile: +66(0)899599453
E-mail: jnac-calibration@jiranatee.com
Web site: www.jiranatee.com

Accredited calibration laboratory
ISO/IEC 17025:2017
NSC-TISI-TIS 17025
CALIBRATION 0367

Air speed measurement laboratory
Calibration services department.

NSC – TISI – TIS 17025
CALIBRATION 0367

Certificate Number
CWS-058-67

CERTIFICATE OF CALIBRATION

REVIEW BY .....

APPROVED BY .....

NEXT CAL DATE 29 Apr 2026

MEASUREMENT ITEM	: Cup anemometer		
MANUFACTURER	: Novalynx		
MODEL/TYPE	: Sensor: WS-02F Data logger: 200-WS-25LB		
SERIAL NUMBER	: Sensor: WSD-A5376 Data logger: A5376		
ID NUMBER	: RYG_FS0414		
CONDITION AS-RECEIVED	: Used item		
CUSTOMER	: ALS laboratory group (Thailand) Co., ltd. 104 Phatthanakan 40, Phatthanakan Rd, Khwaeng Suan Luang, Khet Suan Luang, Bangkok 10250 Thailand.		
RECEIVED DATE	: 18 Oct 2024		
MEASUREMENT DATE	: 29 Oct 2024		
ISSUE DATE	: 29 Oct 2024		
ENVIRONMENTAL CONDITIONS:			
Ambient condition in the laboratory are as follow:			
Temperature	: 23.0 ± 3.0	°C	
Relative Humidity	: 55.0 ± 15.0	%RH	
Atmospheric Pressure	: 1010± 10	hPa	
PLACE OF CALIBRATION	: Eiffel-type wind tunnel of Jiranatee Associates Co., Ltd.		
CALIBRATION CONDITIONS	: Wind tunnel cross-section area[1]	900	cm^2
	Wind direction frontal area[2]	100	cm^2
	Diameter of mounting pipe[3]	-	mm
	Blockage ratio of test object[4]	0.111	[-]
Preconditioning	: 24 hours at ambient conditions.		
Measurement Condition	: The average values during measurement are (23.0) °C, (46.8) %RH and (1003.6) hPa.		

Calibration procedure:

The Cup anemometer was calibrated against Standard air velocity transducer model: 8455-12 and pitot tube with precision differential pressure meter model: DPM2500 in an close test-section of Eiffel-type wind tunnel with 900 cm^2 cross test section area. The WI-CL-007 based on IEC 61400-12-1, Wind energy generation systems – Part 12-1: Power performance measurements of electricity producing wind turbines, March 2017 was used as a calibration guideline.

Traceability:

This certificate provides a traceability of The measurement to recognized the national standards, and to realization of the international system of units (SI) through the NIMT (National Metrology Institute of Thailand) via certificate number: MW-0059-24 and MW-0065-24

Uncertainty of Measurement:

The reported uncertainty of measurement is based on the standard uncertainty multiplied by a coverage factor k=2, Which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty has been determined in accordance with the GUM 'Evaluation of measurement data - Guide to the expression of uncertainty in measurement'

TABULATION OF RESULTS:

The table on next page give the measured values.

Calibrated by:

☑ Mr. Sorawit Thachalad

☐ Miss Jittraporn Lertsomphol

Approved signatory: .....

Mr. Parinya Booncharoen
Calibration Department Manager

Remark:

[1] Nozzle cross-section area of the wind tunnel

[2] Projected cross-section area of the tested object include mounting pipe

[3] Diameter of mounting pipe

[4] Ratio [2] to [1]

THIS CERTIFICATE OF CALIBRATION MAY NOT BE REPRODUCED EXCEPT IN FULL UNLESS PERMISSION FOR REPRODUCTION HAS BEEN OBTAINED IN WRITING FROM THE LABORATORY

Certificate Number
CWS-058-67

MEASUREMENT RESULTS [1]

The Cup anemometer, Unit Under Calibration (UUC) was exercise at 10 m/s for 5 minutes prior to calibration being performed. The standard air velocity 0.5 m/s to 5 m/s was calculated by a standard air velocity transducer which was installed 50 mm away from wind tunnel nozzle and installed 40 mm away from top of the test section and the standard air velocity 5 m/s to 30 m/s was calculated by a pitot tube with precision differential pressure meter which was installed 50 mm away from wind tunnel nozzle and installed 40 mm away from top of the test section, UUC was mounted on a round vertical tube at the lower plate at center of test section. The calibration was carried out under both rising and falling air velocity in the range of 1 m/s to 16 m/s at calibration interval of 1 m/s. The results of calibration and associated measurement uncertainties are reported in the table below.

V_{ref} [2] (m/s)	Temp. wind tunnel (°C)	Temp. room (°C)	V_{unc} [3] (m/s)	Error (m/s)	U (k=2) (m/s)
1.012	22.94	22.95	0.8	-0.2	0.31
2.209	23.00	22.95	2.0	-0.2	0.31
3.050	22.78	22.95	2.9	-0.1	0.31
4.206	22.82	22.95	4.1	0.1	0.31
4.93	22.90	22.95	5.1	0.2	0.31
5.92	22.90	22.95	6.0	0.1	0.31
7.04	22.60	22.95	7.0	-0.1	0.31
7.96	22.74	22.95	8.0	0.1	0.46
8.96	22.76	22.95	8.9	0.0	0.31
9.96	22.50	22.95	10.0	0.1	0.31
11.08	22.90	22.95	11.1	0.0	0.31
12.01	22.52	22.95	12.0	0.0	0.31
12.96	22.58	22.95	13.1	0.1	0.35
13.94	22.54	22.95	14.0	0.1	0.35
14.98	22.60	22.95	15.0	0.0	0.31
15.98	22.60	22.95	16.1	0.1	0.31

Remark:

[1] Calibration results only count for the tested circumstances and environmental conditions during which calibration took place

[2] Velocity of standard

[3] Velocity of Unit Under Calibration

PHOTO OF CALIBRATION SET-UP



Calibration set-up of the Cup anemometer calibration in the wind tunnel of Jiranatee Associates Co., Ltd. The Cup anemometer shown may differ from the calibrated one. Remark: The proportion of the set- up is not true to scale due to imaging geometry.

End of Certificate of Calibration

JIRANATEE ASSOCIATES CO.,LTD.

Jiranatee Associates Co., Ltd.

JIRANATEE ASSOCIATES CO.,LTD.

Jiranatee Associates Co.,Ltd
63/14-15, 67/35-36
Petchkasem 7,7/1, Rd. Watthaya, Bangkokyai,
Bangkok 10600(Thailand)
Tel: +66(0)868308312
Mobile: +66(0)899599453
E-mail: jnac-calibration@jiranatee.com
Web site: www.jiranatee.com

Accredited calibration laboratory
ISO/IEC 17025:2017
NSC-TISI-TIS 17025
CALIBRATION 0367

Air speed measurement laboratory
Calibration services department.

NSC – TISI – TIS 17025
CALIBRATION 0367

Certificate Number
CWS-022-68

CERTIFICATE OF CALIBRATION

REVIEW BY .....

APPROVED BY .....

NEXT CAL DATE 01/02/27

MEASUREMENT ITEM	: Cup anemometer		
MANUFACTURER	: Novalynx		
MODEL/TYPE	: Sensor: WS-02F Data logger: 200-WS-25LB		
SERIAL NUMBER	: Sensor: WSD-A5261 Data logger: A5261		
ID NUMBER	: BKK_FS0888		
CONDITION AS-RECEIVED	: Used item		
CUSTOMER	: ALS laboratory group (Thailand) Co., Ltd. 104 Phatthanakan 40, Phatthanakan Rd, Khwaeng Suan Luang, Khet Suan Luang, Bangkok 10250 Thailand.		
RECEIVED DATE	: 25 Jul 2025		
MEASUREMENT DATE	: 01 Aug 2025		
ISSUE DATE	: 01 Aug 2025		
ENVIRONMENTAL CONDITIONS:			
Ambient condition in the laboratory are as follow:			
Temperature	: 23.0 ± 3.0	°C	
Relative Humidity	: 55.0 ± 15.0	%RH	
Atmospheric Pressure	: 1010± 10	hPa	
PLACE OF CALIBRATION	: Eiffel-type wind tunnel of Jiranatee Associates Co., Ltd.		
CALIBRATION CONDITIONS	: Wind tunnel cross-section area[1]	900	cm^2
	Cup anemometer frontal area[2]	100	cm^2
	Diameter of mounting pipe[3]	-	mm
	Blockage ratio of test object[4]	0.111	[-]
Preconditioning	: 24 hours at ambient conditions.		
Measurement Condition	: The average values during measurement are (24.5) °C, (55.2) %RH and (1005.3) hPa.		

Calibration procedure:

The Cup anemometer was calibrated against Standard air velocity transducer model: 8455-12 and pitot tube with precision differential pressure meter model: DPM2500 in an close test-section of Eiffel-type wind tunnel with 900 cm^2 cross test section area. The WI-CL-007 based on IEC 61400-12-1, Wind energy generation systems – Part 12-1: Power performance measurements of electricity producing wind turbines, March 2017 was used as a calibration guideline.

Traceability:

This certificate provides a traceability of The measurement to recognized the national standards, and to realization of the international system of units (SI) through the NIMT (National Metrology Institute of Thailand) via Certificate number: MW-0019-25 and MW-0065-24

Uncertainty of Measurement:

The reported uncertainty of measurement is based on the standard uncertainty multiplied by a coverage factor k=2, Which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty has been determined in accordance with the GUM 'Evaluation of measurement data - Guide to the expression of uncertainty in measurement'

TABULATION OF RESULTS:

The table on next page give the measured values.

Calibrated by:

☑ Mr. Sorawit Thachalad

☐ Miss Jittraporn Lertsomphol

Approved signatory: .....

Mr. Parinya Booncharoen
Calibration Department Manager

Remark:

[1] Nozzle cross-section area of the wind tunnel

[2] Projected cross-section area of the tested object include mounting pipe

[3] Diameter of mounting pipe

[4] Ratio [2] to [1]

THIS CERTIFICATE OF CALIBRATION MAY NOT BE REPRODUCED EXCEPT IN FULL UNLESS PERMISSION FOR REPRODUCTION HAS BEEN OBTAINED IN WRITING FROM THE LABORATORY

Certificate Number
CWS-022-68

MEASUREMENT RESULTS [1]

The Cup anemometer, Unit Under Calibration (UUC) was exercise at 10 m/s for 1 minutes prior to calibration being performed. The standard air velocity 0.5 m/s to 5 m/s was calculated by a standard air velocity transducer which was installed 50 mm away from wind tunnel nozzle and installed 40 mm away from top of the test section and the standard air velocity 5 m/s to 30 m/s was calculated by a pitot tube with precision differential pressure meter which was installed 50 mm away from wind tunnel nozzle and installed 40 mm away from top of the test section, UUC was mounted on a round vertical tube at the lower plate at center of test section. The calibration was carried out under both rising and falling air velocity in the range of 1 m/s to 16 m/s at calibration interval of 1 m/s. The results of calibration and associated measurement uncertainties are reported in the table below.

V_{ref} [2] (m/s)	Temp. wind tunnel (°C)	Temp. room (°C)	V_{unc} [3] (m/s)	Error (m/s)	U (k=2) (m/s)
1.000	24.38	24.45	0.8	-0.2	0.31
2.256	24.50	24.45	2.0	-0.3	0.31
3.056	24.50	24.45	3.0	-0.1	0.31
4.254	24.48	24.45	4.0	-0.3	0.31
4.94	24.20	24.45	4.8	-0.2	0.31
6.00	24.66	24.45	5.9	-0.1	0.31
7.01	24.30	24.45	7.0	0.0	0.31
7.99	24.70	24.45	8.0	0.0	0.31
9.00	24.30	24.45	9.0	0.0	0.31
10.00	24.70	24.45	10.1	0.1	0.31
11.00	24.04	24.45	11.1	0.1	0.31
11.99	24.64	24.45	12.2	0.2	0.31
12.98	24.12	24.45	13.3	0.3	0.31
14.04	24.52	24.45	14.3	0.3	0.31
15.04	24.22	24.45	15.3	0.3	0.35
16.02	24.34	24.45	16.3	0.3	0.31

Remark:

[1] Calibration results only count for the tested circumstances and environmental conditions during which calibration took place

[2] Velocity of standard

[3] Velocity of Unit Under Calibration

PHOTO OF CALIBRATION SET-UP



Calibration set-up of the Cup anemometer calibration in the wind tunnel of Jiranatee Associates Co., Ltd. The Cup anemometer shown may differ from the calibrated one. Remark: The proportion of the set- up is not true to scale due to imaging geometry.

End of Certificate of Calibration

JIRANATEE ASSOCIATES CO.,LTD.

Jiranatee Associates Co., Ltd.

JIRANATEE ASSOCIATES CO.,LTD.

Jiranatee Associates Co.,Ltd
63/14-15, 67/35-36
Petchkasem 7,7/1, Rd. Watthaya, Bangkokyai,
Bangkok 10600(Thailand)
Tel: +66(0)868308312
Mobile: +66(0)899599453
E-mail: jnac-calibration@jiranatee.com
Web site: www.jiranatee.com

Accredited calibration laboratory
ISO/IEC 17025:2017
NSC-TISI-TIS 17025
CALIBRATION 0367

Wind direction measurement laboratory
Calibration services department.

NSC – TISI – TIS 17025
CALIBRATION 0367

Certificate Number
CWD-022-68

CERTIFICATE OF CALIBRATION

MEASUREMENT ITEM	: Wind Direction Sensor		
MANUFACTURER	: Novalynx		
MODEL/TYPE	: Sensor: WS-02F Data logger: 200-WS-25LB		
SERIAL NUMBER	: Sensor: WSD- A5261 Data logger: A5261		
ID NUMBER	: BKK_FS0888		
CONDITION AS-RECEIVED	: Used item		
CUSTOMER	: ALS laboratory group (Thailand) Co., ltd. 104 Phatthanakan 40, Phatthanakan Rd, Khwaeng Suan Luang, Khet Suan Luang, Bangkok 10250 Thailand.		
RECEIVED DATE	: 25 Jul 2025		
MEASUREMENT DATE	: 01 Aug 2025		
ISSUE DATE	: 01 Aug 2025		
ENVIRONMENTAL CONDITIONS:			
Ambient condition in the laboratory are as follow:			
Temperature	: 23.0 ± 3.0	°C	
Relative Humidity	: 55.0 ± 15.0	%RH	
Atmospheric Pressure	: 1010 ± 10	hPa	
PLACE OF CALIBRATION	: Eiffel-type wind tunnel of Jiranatee Associates Co., Ltd.		
CALIBRATION CONDITION	: Wind tunnel cross-section area[1]	900	cm^2
	Wind direction frontal area[2]	129	cm^2
	Diameter of mounting pipe[3]	-	mm
	Blockage ratio of test object[4]	0.143	[-]
Preconditioning	: 24 hours at ambient conditions.		
Measurement Condition	: The average values during measurement are (23.9)°C, (51.2) %RH and (1003.3) hPa.		

Calibration procedure:

The wind direction sensor was calibrated against Standard Rotary Encoder, model: AX4003T5-DMX4-P3-S-00 in an close test-section of Eiffel-type wind tunnel with 900 cm^2 cross test section area. The WI-CL-008 based on IEC 61400-12-1, Wind energy generation systems – Part 12-1: Power performance measurements of electricity producing wind turbines, March 2017 was used as a calibration guideline.

Traceability:

This certificate provides a traceability of The measurement to recognized the national standards, and to realization of the international system of units (SI) through the NIMT (National Metrology Institute of Thailand) via Certificate number: 04-0027-24.

Uncertainty of Measurement:

The reported uncertainty of measurement is based on the standard uncertainty multiplied by a coverage factor k=2, Which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty has been determined in accordance with the GUM 'Evaluation of measurement data - Guide to the expression of uncertainty in measurement'

TABULATION OF RESULTS:

The table on next page give the measured values.

Calibrated by:

☐ Mr. Sorawit Thachalad

☑ Miss Jittraporn Lertsomphol

Approved signatory: .....

Mr. Parinya Booncharoen
Calibration Department Manager

Remark:

[1] Nozzle cross-section area of the wind tunnel

[2] Projected cross-section area of the tested object include mounting pipe

[3] Diameter of mounting pipe

[4] Ratio [2] to [1]

THIS CERTIFICATE OF CALIBRATION MAY NOT BE REPRODUCED EXCEPT IN FULL UNLESS PERMISSION FOR REPRODUCTION HAS BEEN OBTAINED IN WRITING FROM THE LABORATORY

Certificate Number
CWD-022-68

MEASUREMENT RESULTS [1]

The wind direction sensor was calibrated against standard rotary encoder by comparison method. During calibration, the measurement was carried out at 45° intervals in clockwise and counterclockwise directions after offset adjustment has been made. The flow speed of wind tunnel (usually 5 m/s) is kept constant while the sensor is rotated around its vertical axis. The results of calibration and associated measurement uncertainties are reported in the table below.

Air speed m/s	θ'_{ref} Degree (°)	θ'_{unc} Degree (°)	Error Degree (°)	U (k=2) Degree (°)
5.00	0.000	0	0	0.80
	45.000	41	-4	0.80
	90.000	86	-4	0.80
	135.000	132	-3	0.80
	180.000	181	1	0.80
	225.000	229	4	0.80
	270.000	275	5	0.80
	315.000	320	5	1.34

Remark:

[1] Calibration results only count for the tested circumstances and environmental conditions during which calibration took place

[2] Direction of standard

[3] Direction of Unit Under Calibration

End of Certificate of Calibration

JIRANATEE ASSOCIATES CO.,LTD.

Jiranatee Associates Co., Ltd.

JIRANATEE ASSOCIATES CO.,LTD.
Jiranatee Associates Co.,Ltd
63/14-15, 67/35-36
Petchkasem 7,7/1, Rd. Wutthayas, Bangkokyai,
Bangkok 10600 (Thailand)
Tel: +6628838812
Mobile: +6686 3599453
E-mail: jnac-calibration@jiranatee.com
Web site: www.jiranatee.com

Accredited calibration laboratory
ISO/IEC 17025:2017
NSC-TISI TIS 17025
CALIBRATION 0367

Temperature measurement laboratory
Calibration services department.

NSC – TISI – TIS 17025
CALIBRATION 0367

CERTIFICATE OF CALIBRATION

Certificate No. : CDT-134-68

MEASUREMENT ITEM	: Data Logger with Temperaturesensor
MANUFACTURER	: Novalynx
MODEL/TYPE	: 200-WS-25LB
SERIAL NUMBER	: A5261
ID NUMBER	: BKK_FS0888
CONDITION AS-RECEIVED	: Used item
CUSTOMER	: ALS laboratory group (thailand) Co., Ltd. 104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Suan Luang, Khet Suan Luang, Bangkok 10250 Thailand.
RECEIVED DATE	: 25 Jul 2025
MEASUREMENT DATE	: 01 Aug 2025
ISSUE DATE	: 01 Aug 2025

ENVIRONMENTAL CONDITIONS:
Ambient condition in the laboratory are as follow:

Temperature	: 23.0 ± 3.0	°C
Relative Humidity	: 55.0 ± 15.0	%RH

NOTED: The certificate is valid only to the item calibrated on date and place of calibration.

TABULATION OF RESULTS:
The table on next page give the measured values.

Calibration procedure:
The temperature calibration was done by in-House calibration method as WI-CL-001 according to comparison method with standard digital temperature indicator and standard temperature probe. The temperature scale use was based on ITS-90.

Traceability:
The measurement results are traceable to the International system of units (SI) through National Institute of Metrology Thailand (NIMT) Certificate number: TT-1013-25, Certificate number: EA-0063-26.

Reference Used During Calibration:
1. Standard Temperature Probe
Model: STS-100 A500, Serial No.: 667682-09, Due date: 9 Apr 2026
2. Digital Temperature Indicator
Model: DTI-1000-A MK II, Serial No.: 671407-00591 Due date: 22 Apr 2026

Uncertainty of Measurement:
The reported uncertainty of measurement is based on the standard uncertainty multiplied by a coverage factor k=2, Which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty has been determined in accordance with the GUM 'Evaluation of measurement data - Guide to the expression of uncertainty in measurement'

Calibrated by:
☐ Mr. Sorawit Thachalad
☑ Miss Jittraporn Lertsomphol
☐ Miss Ruangrumpai Phoommit

Approved signatory: .....
Mr. Parinya Boorcharoen
Calibration Department Manager

THIS CERTIFICATE MAY NOT BE REPRODUCED EXCEPT IN FULL UNLESS PERMISSION FOR REPRODUCTION HAS BEEN OBTAINED IN WRITING FROM THE LABORATORY

Result of Calibration: ☑ Without Adjustment ☐ With Adjustment

Calibration Range: 30 °C to 40 °C

Function:

Table 1: This equipment was connected with temperature sensor Model: HMP60 S/N: N0330783. Dimension: Diameter 12 mm. Length 80 mm.

Immersion Depth (mm)	Standard Reading (°C)	UUC Reading (°C)	Error (°C)	Uncertainty (°C)
80	20.057	20.3	0.2	0.099
80	25.044	25.4	0.4	0.099
80	30.027	30.3	0.3	0.099
80	35.011	35.3	0.3	0.099
80	39.996	40.3	0.3	0.099

UUC*: Unit Under Calibration

End of Certificate of Calibration

JIRANATEE ASSOCIATES CO.,LTD.
Jiranatee Associates Co.,Ltd
63/14-15, 67/35-36
Petchkasem 7,7/1, Rd. Wutthayas, Bangkokyai,
Bangkok 10600 (Thailand)
Tel: +6628838812
Mobile: +6686 3599453
E-mail: jnac-calibration@jiranatee.com
Web site: www.jiranatee.com

Accredited calibration laboratory
ISO/IEC 17025:2017
NSC-TISI TIS 17025
CALIBRATION 0367

Relative humidity and Air Temperature measurement laboratory
Calibration services department.

NSC – TISI – TIS 17025
CALIBRATION 0367

CERTIFICATE OF CALIBRATION

Certificate No. : CRT-019-68

MEASUREMENT ITEM	: Relative humidity with data logger
MANUFACTURER	: Novalynx
MODEL/TYPE	: Data Logger: 200-WS-25LB Sensor: HMP60
SERIAL NUMBER	: Data Logger: A5261 Sensor: N0330783
ID NUMBER	: BKK_FS0888
CONDITION AS-RECEIVED	: Used item
CUSTOMER	: ALS laboratory group (Thailand) Co., Ltd. 104 Phatthanakan 40, Phatthanakan Rd, Khwaeng Suan Luang, Khet Suan Luang, Bangkok 10250 Thailand.
RECEIVED DATE	: 25 Jul 2025
MEASUREMENT DATE	: 01 Aug 2025
ISSUE DATE	: 04 Aug 2025

ENVIRONMENTAL CONDITIONS:
Ambient condition in the laboratory are as follow:

Temperature	: 23.0 ± 3.0	°C
Relative Humidity	: 55.0 ± 15.0	%RH

NOTED: The certificate is valid only to the item calibrated on date and place of calibration.

TABULATION OF RESULTS:
The table on next page give the measured values.

Calibration procedure:
The Relative humidity and Air Temperature calibration was done by in-House calibration method as WI-CL-009 and WI-CL-010 according to comparison method with Standard Chilled Mirror hygrometer with Temperature sensor and standard Humidity generator chamber.

Traceability:
The measurements are traceable to the International System of Units (SI) through National Institute of Metrology Thailand (NIMT). Certificate number: TH-0146-24 and Jiranatee Associates Co., Ltd. Certificate number: CDT-026-68.

Uncertainty of Measurement:
The reported uncertainty of measurement is based on the standard uncertainty multiplied by a coverage factor k=2, Which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty has been determined in accordance with the GUM 'Evaluation of measurement data - Guide to the expression of uncertainty in measurement'

Calibrated by:
☐ Mr. Sorawit Thachalad
☑ Miss Jittraporn Lertsomphol
☐ Miss Ruangrumpai Phoommit

Approved signatory: .....
Mr. Parinya Boorcharoen
Calibration Department Manager

THIS CERTIFICATE OF CALIBRATION MAY NOT BE REPRODUCED EXCEPT IN FULL UNLESS PERMISSION FOR REPRODUCTION HAS BEEN OBTAINED IN WRITING FROM THE LABORATORY

Measurement Results:

The results of calibration and associated measurement uncertainties are reported in the table below.

Result of Calibration: ☑ Without Adjustment ☐ With Adjustment

Table 1: The results of calibration of relative humidity at 30 °C are reported in table below.
Calibration Range: 20%RH to 80%RH

Air Temperature (°C)	Standard Reading (%RH)	UUC Reading (%RH)	Error (%RH)	Uncertainty ± (%RH)
30.06	20.04	19.1	-0.9	0.78
30.05	50.13	49.3	-0.9	1.3
30.08	80.14	18.8	-1.3	2.1

UUC*: Unit Under Calibration

End of Certificate of Calibration

JIRANATEE ASSOCIATES CO.,LTD.
Jiranatee Associates Co.,Ltd
63/14-15, 67/35-36
Petchkasem 7,7/1, Rd. Wutthayas, Bangkokyai,
Bangkok 10600 (Thailand)
Tel: +6628838812
Mobile: +6686 3599453
E-mail: jnac-calibration@jiranatee.com
Web site: www.jiranatee.com

Accredited calibration laboratory
ISO/IEC 17025:2017
NSC-TISI TIS 17025
CALIBRATION 0367

Air speed measurement laboratory
Calibration services department.

NSC – TISI – TIS 17025
CALIBRATION 0367

Certificate Number
CWS-055-67

CERTIFICATE OF CALIBRATION

REVIEW BY .....
APPROVED BY .....
NEXT CAL DATE..... 29 Apr 2026

MEASUREMENT ITEM	: Cup anemometer
MANUFACTURER	: Novalynx
MODEL/TYPE	: Sensor: WS-02F Data logger: 200-WS-25LB
SERIAL NUMBER	: Sensor: WSD-A5369 Data logger: A5369
ID NUMBER	: RYO_FS0411
CONDITION AS-RECEIVED	: Used item
CUSTOMER	: ALS laboratory group (Thailand) Co., Ltd. 104 Phatthanakan 40, Phatthanakan Rd, Khwaeng Suan Luang, Khet Suan Luang, Bangkok 10250 Thailand.
RECEIVED DATE	: 18 Oct 2024
MEASUREMENT DATE	: 29 Oct 2024
ISSUE DATE	: 29 Oct 2024

ENVIRONMENTAL CONDITIONS:
Ambient condition in the laboratory are as follow:

Temperature	: 23.0 ± 3.0	°C
Relative Humidity	: 55.0 ± 15.0	%RH
Atmospheric Pressure	: 1010± 10	hPa

PLACE OF CALIBRATION : Eiffel-type wind tunnel of Jiranatee Associates Co., Ltd.

CALIBRATION CONDITIONS

Wind tunnel cross-section area[1]	900	cm^2
Wind direction frontal area[2]	100	cm^2
Diameter of mounting pipe[3]	-	mm
Blockage Ratio of test object[4]	0.111	[-]

Preconditioning : 24 hours at ambient conditions.
Measurement Condition : The average values during measurement are (24.0) °C, (61.0) %RH and (1005.4) hPa.

Calibration procedure:
The Cup anemometer was calibrated against Standard air velocity transducer model: 8455-02 and pitot tube with precision differential pressure meter model: DPM2500 in an close test section of Eiffel-type wind tunnel with 900 cm^2 cross test section area. The WI-CL-007 based on IEC 61400-12-1, Wind energy generation systems – Part 12-1: Power performance measurements of electricity producing wind turbines, March 2017 was used as a calibration guideline.

Traceability:
This certificate provides a traceability of The measurement to recognized the national standards, and to realization of the international system of units (SI) through the NIMT (National Metrology Institute of Thailand) via Certificate number: MAY-0003-24 and MAY-0065-24

Uncertainty of Measurement:
The reported uncertainty of measurement is based on the standard uncertainty multiplied by a coverage factor k=2, Which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty has been determined in accordance with the GUM 'Evaluation of measurement data - Guide to the expression of uncertainty in measurement'

TABULATION OF RESULTS:
The table on next page give the measured values.

Calibrated by:
☑ Mr. Sorawit Thachalad
☐ Miss Jittraporn Lertsomphol

Approved signatory: .....
Mr. Parinya Boorcharoen
Calibration Department Manager

Remark:
[1] Nozzle cross-section area of the wind tunnel
[2] Projected cross-section area of the tested object include mounting pipe
[3] Diameter of mounting pipe
[4] Ratio $^1/_{10}$

THIS CERTIFICATE OF CALIBRATION MAY NOT BE REPRODUCED EXCEPT IN FULL UNLESS PERMISSION FOR REPRODUCTION HAS BEEN OBTAINED IN WRITING FROM THE LABORATORY

Certificate Number
CWS-055-67

MEASUREMENT RESULTS [5]

The Cup anemometer, Unit Under Calibration (UUC) was exercise at 10 m/s for5 minutes prior to calibration being performed. The standard air velocity 0.5 m/s to 5 m/s was calculated by a standard air velocity transducer which was installed 50 mm away from wind tunnel nozzle and installed 40 mm away from top of the test section and the standard air velocity 5 m/s to 30 m/s was calculated by a pitot tube with precision differential pressure meter which was installed 50 mm away from wind tunnel nozzle and installed 40 mm away from top of the test section, UUC was mounted on a round vertical tube of the lower plate at center of test section. The calibration was carried out under both rising and falling air velocity in the range of 1 m/s to 16 m/s at calibration interval of 1 m/s. The results of calibration and associated measurement uncertainties are reported in the table below.

v_{ref} [2] (m/s)	Temp. wind tunnel (°C)	Temp. room (°C)	v_{uut} [3] (m/s)	Error (m/s)	U (k=2) (m/s)
1.020	23.56	24.00	0.8	-0.2	0.31
2.225	24.50	24.00	2.0	-0.2	0.31
3.086	23.74	24.00	3.0	-0.1	0.31
4.269	23.72	24.00	4.0	-0.3	0.31
4.95	23.76	24.00	5.0	0.0	0.31
5.96	23.78	24.00	6.0	0.0	0.31
7.03	23.70	24.00	7.1	0.0	0.31
7.96	23.60	24.00	7.9	-0.1	0.31
8.95	23.80	24.00	8.9	-0.1	0.31
9.95	23.52	24.00	10.0	0.1	0.31
11.08	23.80	24.00	11.2	0.1	0.31
12.02	23.66	24.00	12.1	0.1	0.31
12.94	23.90	24.00	13.2	0.2	0.31
13.93	23.70	24.00	14.2	0.3	0.31
14.97	23.90	24.00	15.3	0.3	0.31
16.01	23.93	24.00	16.5	0.4	0.31

Remark:
[1] Calibration results only count for the tested circumstances and environmental conditions during which calibration took place
[2] Velocity of standard
[3] Velocity of Unit Under Calibration

PHOTO OF CALIBRATION SET-UP



Calibration set-up of the Cup anemometer calibration in the wind tunnel of Jiranatee Associates Co., Ltd. The Cup anemometer shown may differ from the calibrated one. Remark: The proportion of the set- up is not true to scale due to imaging geometry.

End of Certificate of Calibration

JIRANATEE ASSOCIATES CO.,LTD.
Jiranatee Associates Co.,Ltd
63/14-15, 67/35-36
Petchkasem 7,7/1, Rd. Wutthayas, Bangkokyai,
Bangkok 10600 (Thailand)
Tel: +6628838812
Mobile: +6686 3599453
E-mail: jnac-calibration@jiranatee.com
Web site: www.jiranatee.com

Accredited calibration laboratory
ISO/IEC 17025:2017
NSC-TISI TIS 17025
CALIBRATION 0367

Air speed measurement laboratory
Calibration services department.

NSC – TISI – TIS 17025
CALIBRATION 0367

Certificate Number
CWS-012-68

CERTIFICATE OF CALIBRATION

MEASUREMENT ITEM	: Cup anemometer
MANUFACTURER	: Novalynx
MODEL/TYPE	: Sensor: WS-02F Data logger: 200-WS-25LB
SERIAL NUMBER	: Sensor: WSD-A4916 Data logger: A4916
ID NUMBER	: BKK_FS0163
CONDITION AS-RECEIVED	: Used item
CUSTOMER	: ALS laboratory group (Thailand) Co., Ltd. 104 Phatthanakan 40, Phatthanakan Rd, Khwaeng Suan Luang, Khet Suan Luang, Bangkok 10250 Thailand.
RECEIVED DATE	: 18 Apr 2025
MEASUREMENT DATE	: 06 May 2025
ISSUE DATE	: 09 May 2025

ENVIRONMENTAL CONDITIONS:
Ambient condition in the laboratory are as follow:

Temperature	: 23.0 ± 3.0	°C
Relative Humidity	: 55.0 ± 15.0	%RH
Atmospheric Pressure	: 1010± 10	hPa

PLACE OF CALIBRATION : Eiffel-type wind tunnel of Jiranatee Associates Co., Ltd.

CALIBRATION CONDITIONS

Wind tunnel cross-section area[1]	900	cm^2
Cup anemometer frontal area[2]	160	cm^2
Diameter of mounting pipe[3]	-	mm
Blockage Ratio of test object[4]	0.111	[-]

Preconditioning : 24 hours at ambient conditions.
Measurement Condition : The average values during measurement are (24.0) °C, (43.2) %RH and (1008.0) hPa.

Calibration procedure:
The Cup anemometer was calibrated against Standard air velocity transducer model: 8455-02 and pitot tube with precision differential pressure meter model: DPM2500 in an close test section of Eiffel-type wind tunnel with 900 cm^2 cross test section area. The IEC 61400-12-1, Wind energy generation systems – Part 12-1: Power performance measurements of electricity producing wind turbines, March 2017 was used as a calibration guideline.

Traceability:
This certificate provides a traceability of The measurement to recognized the national standards, and to realization of the international system of units (SI) through the NIMT (National Metrology Institute of Thailand) via Certificate number: MAY-0003-25 and MAY-0055-24

Uncertainty of Measurement:
The reported uncertainty of measurement is based on the standard uncertainty multiplied by a coverage factor k=2, Which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty has been determined in accordance with the GUM 'Evaluation of measurement data - Guide to the expression of uncertainty in measurement'

REVIEW BY .....
APPROVED BY .....
NEXT CAL DATE..... 06/11/26

TABULATION OF RESULTS:
The table on next page give the measured values.

Calibrated by:
☐ Mr. Sorawit Thachalad
☑ Miss Jittraporn Lertsomphol

Approved signatory: .....
Mr. Parinya Boorcharoen
Calibration Department Manager

Remark:
[1] Nozzle cross-section area of the wind tunnel
[2] Projected cross-section area of the tested object include mounting pipe
[3] Diameter of mounting pipe
[4] Ratio $^1/_{10}$

THIS CERTIFICATE OF CALIBRATION MAY NOT BE REPRODUCED EXCEPT IN FULL UNLESS PERMISSION FOR REPRODUCTION HAS BEEN OBTAINED IN WRITING FROM THE LABORATORY

Certificate Number
CWS-012-68


MEASUREMENT RESULTS [5]

The Cup anemometer, Unit Under Calibration (UUC) was exercise at 10 m/s for 5minutes prior to calibration being performed. The standard air velocity 0.5 m/s to 5 m/s was calculated by a standard air velocity transducer which was installed 50 mm away from wind tunnel nozzle and installed 40 mm away from top of the test section and the standard air velocity 5 m/s to 30 m/s was calculated by a pitot tube with precision differential pressure meter which was installed 50 mm away from wind tunnel nozzle and installed 40 mm away from top of the test section, UUC was mounted on a round vertical tube of the lower plate at center of test section. The calibration was carried out under both rising and falling air velocity in the range of 1 m/s to 16 m/s at calibration interval of 1 m/s. The results of calibration and associated measurement uncertainties are reported in the table below.

v_{ref} [2] (m/s)	Temp. wind tunnel (°C)	Temp. room (°C)	v_{uut} [3] (m/s)	Error (m/s)	U (k=2) (m/s)
1.020	23.92	23.95	0.9	-0.1	0.31
2.282	24.10	23.95	2.0	-0.3	0.31
3.125	24.10	23.95	3.0	-0.1	0.31
4.316	24.08	23.95	4.0	-0.4	0.31
4.96	24.10	23.95	5.0	0.0	0.31
5.96	24.34	23.95	6.0	0.1	0.31
7.04	24.02	23.95	7.1	0.1	0.31
7.96	24.18	23.95	8.1	0.1	0.31
9.01	23.92	23.95	9.1	0.1	0.31
10.01	23.92	23.95	10.3	0.3	0.31
11.03	24.00	23.95	11.2	0.2	0.31
11.99	23.80	23.95	12.2	0.2	0.31
12.98	24.04	23.95	13.3	0.4	0.31
14.00	23.86	23.95	14.4	0.4	0.31
15.02	24.08	23.95	15.4	0.4	0.31
16.05	23.98	23.95	16.4	0.4	0.31

Remark:
[1] Calibration results only count for the tested circumstances and environmental conditions during which calibration took place
[2] Velocity of standard
[3] Velocity of Unit Under Calibration

PHOTO OF CALIBRATION SET-UP



Calibration set-up of the Cup anemometer calibration in the wind tunnel of Jiranatee Associates Co., Ltd. The Cup anemometer shown may differ from the calibrated one. Remark: The proportion of the set- up is not true to scale due to imaging geometry.

End of Certificate of Calibration

JIRANATEE ASSOCIATES CO.,LTD.
Jiranatee Associates Co.,Ltd
63/14-15, 67/35-36
Petchkasem 7,7/1, Rd. Wutthayas, Bangkokyai,
Bangkok 10600 (Thailand)
Tel: +6628838812
Mobile: +6686 3599453
E-mail: jnac-calibration@jiranatee.com
Web site: www.jiranatee.com

Accredited calibration laboratory
ISO/IEC 17025:2017
NSC-TISI TIS 17025
CALIBRATION 0367

Wind direction measurement laboratory
Calibration services department.

NSC – TISI – TIS 17025
CALIBRATION 0367

Certificate Number
CWD-012-68

CERTIFICATE OF CALIBRATION

MEASUREMENT ITEM	: Wind Direction Sensor
MANUFACTURER	: Novalynx
MODEL/TYPE	: Sensor: WS-02F Data logger: 200-WS-25LB
SERIAL NUMBER	: Sensor: WSD-A4916 Data logger: A4916
ID NUMBER	: BKK_FS0163
CONDITION AS-RECEIVED	: Used item
CUSTOMER	: ALS laboratory group (Thailand) Co., Ltd. 104 Phatthanakan 40, Phatthanakan Rd, Khwaeng Suan Luang, Khet Suan Luang, Bangkok 10250 Thailand.
RECEIVED DATE	: 18 Apr 2025
MEASUREMENT DATE	: 06 May 2025
ISSUE DATE	: 09 May 2025

ENVIRONMENTAL CONDITIONS:
Ambient condition in the laboratory are as follow:

Temperature	: 23.0 ± 3.0	°C
Relative Humidity	: 55.0 ± 15.0	%RH
Atmospheric Pressure	: 1010 ± 10	hPa

PLACE OF CALIBRATION : Eiffel-type wind tunnel of Jiranatee Associates Co., Ltd.

CALIBRATION CONDITION

Wind tunnel cross-section area[1]	900	cm^2
Wind direction frontal area[2]	129	cm^2
Diameter of mounting pipe[3]	-	mm
Blockage Ratio of test object[4]	0.143	[-]

Preconditioning : 24 hours at ambient conditions.
Measurement Condition : The average values during measurement are (24.1)°C, (42.0) %RH and (1005.2) hPa.

Calibration procedure:
The wind direction sensor was calibrated against Standard Rotary Encoder model: AS05225D-BMSM-F3-5-ENV in an close test section of Eiffel-type wind tunnel with 900 cm^2 cross test section area. The WI-CL-008 based on IEC 61400-12-1, Wind energy generation systems – Part 12-1: Power performance measurements of electricity producing wind turbines, March 2017 was used as a calibration guideline.

Traceability:
This certificate provides a traceability of The measurement to recognized the national standards, and to realization of the international system of units (SI) through the NIMT (National Metrology Institute of Thailand) via Certificate number: MAY-0003-24.

Uncertainty of Measurement:
The reported uncertainty of measurement is based on the standard uncertainty multiplied by a coverage factor k=2, Which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty has been determined in accordance with the GUM 'Evaluation of measurement data - Guide to the expression of uncertainty in measurement'

TABULATION OF RESULTS:
The table on next page give the measured values.

Calibrated by:
☐ Mr. Sorawit Thachalad
☑ Miss Jittraporn Lertsomphol

Approved signatory: .....
Mr. Parinya Boorcharoen
Calibration Department Manager

Remark:
[1] Nozzle cross-section area of the wind tunnel
[2] Projected cross-section area of the tested object include mounting pipe
[3] Diameter of mounting pipe
[4] Ratio $^1/_{10}$

THIS CERTIFICATE OF CALIBRATION MAY NOT BE REPRODUCED EXCEPT IN FULL UNLESS PERMISSION FOR REPRODUCTION HAS BEEN OBTAINED IN WRITING FROM THE LABORATORY

Certificate Number
CWD-012-68

MEASUREMENT RESULTS [5]

The wind direction sensor was calibrated against standard rotary encoder by comparison method. During calibration, the measurement was carried out at 45° intervals in clockwise and counterclockwise directions after offset adjustment has been made. The flow speed of wind tunnel (usually 5 m/s) is kept constant while the sensor is rotated around its vertical axis. The results of calibration and associated measurement uncertainties are reported in the table below.

Air speed	D'_{set}	D'_{acc}	Error	U (k=2)
m/s	Degree (°)	Degree (°)	Degree (°)	Degree (°)
5.01	45.000	42	-3	0.80
	90.000	87	-3	0.80
	135.000	133	-2	0.80
	180.000	180	0	0.80
	225.000	227	2	0.80
	270.000	273	3	0.80
	315.000	318	3	0.80
	360.000	359	-1	0.80

Remark:

[4] Calibration results only meant for the tested circumstances and environmental conditions during which calibration took place

[4] Direction of standard

[5] Direction of Unit Under Calibration

End of Certificate of Calibration

Jiranatee Associates Co., Ltd.

JIRANATEE ASSOCIATES CO.,LTD.

Jiranatee Associates Co.,Ltd
63/14 15, 17/35-36
Petchkasem 7, 7/1, Rd, Wattthapra, Bangkokyai,
Bangkok 10600 (Thailand)
Tel: +66(0)818381317
Mobile: +66(0)1919453
E-mail: jiranatee@jiranatee.com
Web site: www.jiranatee.com

Accredited calibration laboratory
ISO/IEC 17025:2017
NSC-TISI-TIS 17025
CALIBRATION 0367

Wind direction measurement laboratory
Calibration services department.

NSC – TISI – TIS 17025
CALIBRATION 0367

Certificate Number
CWD-061-67

CERTIFICATE OF CALIBRATION

MEASUREMENT ITEM	: Wind Direction Sensor	
MANUFACTURER	: Novalynx	
MODEL/TYPE	: Sensor: WS-02F	
	Data logger: 200-WS-25LB	
SERIAL NUMBER	: Sensor: WSD-A5377	
	Data logger: A5377	
ID NUMBER	: BKK_FS0917	
CONDITION AS RECEIVED	: Used item	
CUSTOMER	: ALS laboratory group (Thailand) Co, Ltd.	
	104 Phatthanakan 40, Phatthanakan Rd, Khwaeng Suan Luang,	
	Khet Suan Luang, Bangkok 10250 Thailand.	
RECEIVED DATE	: 22 Nov 2024	
MEASUREMENT DATE	: 25 Nov 2024	
ISSUE DATE	: 25 Nov 2024	
ENVIRONMENTAL CONDITIONS:		
Ambient condition in the laboratory are as follow:		
Temperature	: 23.0 ± 3.0	°C
Relative Humidity	: 55.0 ± 15.0	%RH
Atmospheric Pressure	: 1010± 10	hPa
PLACE OF CALIBRATION	: Eiffel-type wind tunnel of Jiranatee Associates Co., Ltd.	
CALIBRATION CONDITION	: Wind tunnel cross-section area[1]	900 cm²
	Wind direction frontal area[2]	100 cm²
	Diameter of mounting pipe[3]	- mm
	Blockage ratio of test object[4]	0.143 [-]
Preconditioning	: 24 hours at ambient conditions.	
Measurement Condition	: The average values during measurement are (23.7)°C, (50.3) %RH and (1019.9)hPa.	
TABULATION OF RESULTS:		
The table on next page give the measured values.		
Calibrated by:	☒ Mr. Sorawit Thapsorn	
	☐ Miss Jittaporn Lertpaisarnsil	

Calibration procedure:
The wind direction sensor was calibrated against Standard Rotary Encoder, model: AS5311P-DMNN-F5-5-ST5 in an close test section of a pilot type wind tunnel with 500 cm² cross test section area. The IEC-61400-12-1, Wind energy generation systems – Part 12-1: Power performance measurements of electricity producing wind turbines, March 2017 was used as a calibration guideline.

Traceability:
This certificate provides a traceability of The measurement to recognized the national standards, and to realization of the international system of units (SI) through the NIMT (National Metrology Institute of Thailand) via Certificate number: 0N-0167-68.

Uncertainty of Measurement:
The reported uncertainty of measurement is based on the standard uncertainty multiplied by a coverage factor k=2, Which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty has been determined in accordance with the GUM 'Evaluation of measurement data - Guide to the expression of uncertainty in measurement'

REVIEW BY ..... Manatsa. P.
APPROVED BY .....
NEXT CAL DATE..... 25/05/26

Approved signatory: .....
Mr. Yanivya Boonchanoon
Calibration Department Manager

Remark:
[1] Nozzle cross-section area of the wind tunnel
[2] Projected cross-section area of the tested object include mounting pipe
[3] Diameter of mounting pipe
[4] Ratio [2] to [1]

THIS CERTIFICATE OF CALIBRATION MAY NOT BE REPRODUCED EXCEPT IN FULL UNLESS PERMISSION FOR REPRODUCTION HAS BEEN OBTAINED IN WRITING FROM THE LABORATORY

Certificate Number
CWD-063-67

MEASUREMENT RESULTS [5]

The wind direction sensor was calibrated against standard rotary encoder by comparison method. During calibration, the measurement was carried out at 45° intervals in clockwise and counterclockwise directions after offset adjustment has been made. The flow speed of wind tunnel (usually 3 m/s) is kept constant while the sensor is rotated around its vertical axis. The results of calibration and associated measurement uncertainties are reported in the table below.

Air speed	D'_{set}	D'_{acc}	Error	U (k=2)
m/s	Degree (°)	Degree (°)	Degree (°)	Degree (°)
5.02	45.000	41	-4	0.80
	90.000	86	-4	0.80
	135.000	132	-3	0.80
	180.000	181	1	0.80
	225.000	229	4	0.80
	270.000	275	5	0.80
	315.000	320	5	0.80
	360.000	359	-1	0.80

Remark:

[4] Calibration results only meant for the tested circumstances and environmental conditions during which calibration took place

[4] Direction of standard

[5] Direction of Unit Under Calibration

End of Certificate of Calibration

Jiranatee Associates Co., Ltd.

JIRANATEE ASSOCIATES CO.,LTD.

Jiranatee Associates Co.,Ltd
63/14 15, 17/35-36
Petchkasem 7, 7/1, Rd, Wattthapra, Bangkokyai,
Bangkok 10600 (Thailand)
Tel: +66(0)818381317
Mobile: +66(0)1919453
E-mail: jnac-calibration@jiranatee.com
Web site: www.jiranatee.com

Accredited calibration laboratory
ISO/IEC 17025:2017
NSC-TISI-TIS 17025
CALIBRATION 0367

Air speed measurement laboratory
Calibration services department.

NSC – TISI – TIS 17025
CALIBRATION 0367

Certificate Number
CWS-061-67

CERTIFICATE OF CALIBRATION

MEASUREMENT ITEM	: Cup anemometer	
MANUFACTURER	: Novalynx	
MODEL/TYPE	: Sensor: WS-02F	
	Data logger: 200-WS-25LB	
SERIAL NUMBER	: Sensor: WSD-A5377	
	Data logger: A5377	
ID NUMBER	: BKK_FS0917	
CONDITION AS RECEIVED	: Used item	
CUSTOMER	: ALS laboratory group (Thailand) Co, Ltd.	
	104 Phatthanakan 40, Phatthanakan Rd, Khwaeng Suan Luang,	
	Khet Suan Luang, Bangkok 10250 Thailand.	
RECEIVED DATE	: 22 Nov 2024	
MEASUREMENT DATE	: 25 Nov 2024	
ISSUE DATE	: 25 Nov 2024	
ENVIRONMENTAL CONDITIONS:		
Ambient condition in the laboratory are as follow:		
Temperature	: 23.0 ± 3.0	°C
Relative Humidity	: 55.0 ± 15.0	%RH
Atmospheric Pressure	: 1010± 10	hPa
PLACE OF CALIBRATION	: Eiffel-type wind tunnel of Jiranatee Associates Co., Ltd.	
CALIBRATION CONDITIONS	: Wind tunnel cross-section area[1]	900 cm²
	Wind direction frontal area[2]	100 cm²
	Diameter of mounting pipe[3]	- mm
	Blockage ratio of test object[4]	0.111 [-]
Preconditioning	: 24 hours at ambient conditions.	
Measurement Condition	: The average values during measurement are (24.9) °C, (43.3) %RH and (1008.2) hPa.	
TABULATION OF RESULTS:		
The table on next page give the measured values.		
Calibrated by:	☒ Mr. Sorawit Thapsorn	
	☐ Miss Jittaporn Lertpaisarnsil	

Calibration procedure:
The Cup anemometer was calibrated against Standard air velocity transducer model: 8455IR2 and pitot tube with precision differential pressure meter model: DPM1703 in accordance with calibration of Eight-type wind tunnels with 900 cm² cross test section area. The IEC-61400-12-1, Wind energy generation systems – Part 12-1: Power performance measurements of electricity producing wind turbines, March 2017 was used as a calibration guideline.

Traceability:
This certificate provides a traceability of The measurement to recognized the national standards, and to realization of the international system of units (SI) through the NIMT (National Metrology Institute of Thailand) via Certificate number: 0N-0107-24 and MID 0365-24

Uncertainty of Measurement:
The reported uncertainty of measurement is based on the standard uncertainty multiplied by a coverage factor k=2, Which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty has been determined in accordance with the GUM 'Evaluation of measurement data - Guide to the expression of uncertainty in measurement'

Approved signatory: .....
Mr. Farinya Boonchanoon
Calibration Department Manager

Remark:
[1] Nozzle cross-section area of the wind tunnel
[2] Projected cross-section area of the tested object include mounting pipe
[3] Diameter of mounting pipe
[4] Ratio [2] to [1]

THIS CERTIFICATE OF CALIBRATION MAY NOT BE REPRODUCED EXCEPT IN FULL UNLESS PERMISSION FOR REPRODUCTION HAS BEEN OBTAINED IN WRITING FROM THE LABORATORY

Certificate Number
CWS-061-67

MEASUREMENT RESULTS [5]

The Cup anemometer, Unit Under Calibration (UUC) was exercise at 10 m/s for 5-minutes prior to calibration being performed. The standard air velocity 0.5 m/s to 5 m/s was calculated by a standard air velocity transducer which was installed 50 mm away from wind tunnel nozzle and installed 40 mm away from top of the test section and the standard air velocity 5 m/s to 30 m/s was calculated by a pitot tube with precision differential pressure meter which was installed 50 mm away from wind tunnel nozzle and installed 40 mm away from top of the test section, UUC was mounted on a round vertical tube of the lower plate at center of test section. The calibration was carried out under both rising and falling air velocity in the range of 1 m/s to 36 m/s at calibration interval of 1 m/s. The results of calibration and associated measurement uncertainties are reported in the table below.

v_{set}[5] (m/s)	Temp. wind tunnel (°C)	Temp. room (°C)	v_{acc}[5] (m/s)	Error (m/s)	U (k=2) (m/s)
1.012	24.30	24.90	0.9	-0.2	0.31
2.218	25.58	24.90	2.0	-0.2	0.31
3.050	24.30	24.90	2.9	-0.1	0.31
4.233	24.30	24.90	4.0	-0.2	0.31
4.94	24.30	24.90	5.0	0.0	0.31
5.98	24.60	24.90	6.0	0.0	0.31
7.03	24.30	24.90	7.2	0.1	0.31
7.96	24.34	24.90	8.1	0.1	0.31
8.97	24.30	24.90	9.0	0.0	0.31
9.97	24.38	24.90	9.9	-0.1	0.31
11.09	24.32	24.90	11.2	0.1	0.31
12.03	24.30	24.90	12.1	0.1	0.31
12.92	24.18	24.90	13.0	0.1	0.33
13.92	24.30	24.90	14.0	0.1	0.31
14.98	24.30	24.90	15.1	0.1	0.31
15.98	24.30	24.90	16.1	0.1	0.35

Remark:

[4] Calibration results only meant for the tested circumstances and environmental conditions during which calibration took place

[4] Velocity of standard

[5] Velocity of Unit Under Calibration

PHOTO OF CALIBRATION SET-UP



Calibration set-up of the Cup anemometer calibration in the wind tunnel of Jiranatee Associates Co., Ltd. The Cup anemometer shown may differ from the calibrated one. Remark: The proportion of the set- up is not true to scale due to imaging geometry.

End of Certificate of Calibration

Jiranatee Associates Co., Ltd.

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7/139 MOO 13, SOI SUNTINAKORN 11 TAMBON BANG KAEO,
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL: 0660-2116-5860-1 FAX: 0660-2116-7140

Certificate of Calibration

Customer

Name	: ALS Laboratory Group Thailand Co., Ltd.	**Certificate No**	: 25-ACT-010
Address	: 104 Soi Phatthanakan 40, Phatthanakan Road, Suan Luang, Bangkok 10250	**Request No**	: Req-2025-0091

Unit Under Calibration Details

Measurement item	: Acoustic Calibrator	Class	: 1
Manufacturer	: RION	Range	: 94 dB / 1000 Hz
Model	: NC-74	Instrument Status	: Used
Serial Number	: 34178121		
ID	: RYG_FS0213		

REVIEW BY ..... Manatsa. P.
APPROVED BY .....
NEXT CAL DATE..... 18/01/26

Calibration Environment and Details

Temperature	: (23 ±2 °C)
Humidity	: (50 ± 20 %RH)
Barometric Pressure	: (1013 ±10.0 hPa)
Received Date	: 15 January 2025
Calibration Date	: 16 January 2025
Location of Calibration	: LAB 1 Acoustic
Calibration Procedure	: In-house method CP-ACT-02 based on IEC 60942:2017 Electroacoustics - Sound calibrators

Reference Standard	Model	Serial Number	Traceable	Due Calibration
Sound Calibrator	SV 35A	58079	EEI	12 June 2025
THD Multimeter	2015	1647765	NIMT	16 January 2025

Traceability : This certificate providoes traceability of measurement to recognized national standard, and to the realization of the international System ofUnits (SI).

Note

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor k =2, providing a level of confidence approximately 95 %.

Calibrated By : Mr. Noppadon Luangart, Service Calibration Engineer

Approved By : Mr. Pacit Mathavorn, Calibration Engineer Supervisor

Issue Date : 16 January 2025

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7/139 MOO 13, SOI SUNTINAKORN 11 TAMBON BANG KAEO,
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL: 0660-2116-5860-1 FAX: 0660-2116-7140

Certificate No : 25-ACT-010
Request No : Req-2025-0091

Sound pressure level — **Calibration Results :** Without Adjustment

Calibration Range	Without Adjustment (dB)		Adjustment (dB)		Uncertainty	Acceptance limit	Result
(dB)	Measured	Deviated value	Measured	Deviated value	(± dB)	Class 1 (± dB)	
94 dB / 1000 Hz	94.11	0.11	-	-	0.13	0.25	Pass

Frequency of Sound pressure level

Calibration Range	Without Adjustment		Adjustment		Uncertainty	Acceptance limit	Result
(Hz)	Measured (Hz)	Deviated	Measured (Hz)	Deviated	(± %)	Class 1 (± %)	
94 dB / 1000 Hz	1000.00	0.00	-	-	0.01	0.70	Pass

Total Harmonic Distortion plus Noise of Sound pressure level (THD+N %)

Calibration Range	Without Adjustment	Adjustment	Uncertainty	Acceptance limit	Result
(Hz)	Measured (%)	Measured (%)	(± %)	Class 1 (± %)	
94 dB / 1000 Hz	1.21	-	0.40	2.5	Pass

Note :

Function	Maximum-permitted Uncertainty of measurement
Sound pressure level	0.15 dB
Frequency	0.20%
Total distortion+noise	0.50%

- Acceptance limit was IEC60942:2017 Class 1
- The calibration results exclude the calibrator pressure correction
- The calibration results exclude the microphone volume correction

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7/139 MOO 13, SOI SUNTINAKORN 11 TAMBON BANG KAEO,
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL: 0660-2116-5860-1 FAX: 0660-2116-7140

Certificate No : 25-ACT-010
Request No : Req-2025-0091

Decision Rule for Statements of Conformity


The standard decision rule employed for the statements of conformity to each calibrationresult will be applied using ILAC-G8:09/2019, Guidelines on the Reporting of Compliance with Specification as following Fig. and statements

Pass = The measurement result plus the expanded uncertainty with a 95% coverage probability were within the limit.

Pass[1] = The measurement result was within the limit. However, a portion of the expanded uncertainty of measurement at 95% exceeds the limit.

Fail[2] = The measurement result was out of the limit. However, a portion of the expanded uncertainty of measurement at 95% is within the limit.

Fail = The measurement result plus the expanded uncertainty with a 95% coverage probability were outside the limit.



End of Calibration

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7/139 MOO 13, SOI SUNTINAKORN 11 TAMBON BANG KAEO,
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL: 0660-2116-5860-1 FAX: 0660-2116-7140

Certificate of Calibration

Customer

Name	: ALS Laboratory Group Thailand Co., Ltd.	**Certificate No :**	25-SLM-114
Address	: 104 Soi Phatthanakan 40, Phatthanakan Road, Suan Luang, Bangkok 10250	**Request No :**	Req-2025-0603

Unit Under Calibration Details

Measurement item :	Sound Level Meter	Microphone Class :	2
Manufacturer	: RION	Microphone Model :	UC-52
Model	: NL-42	Microphone S/N :	143811
Serial Number	: 01222723	Preamplifier Model :	NH-24
ID	: RYG_FS0022	Preamplifier S/N :	22770
Resolution	: 0.1 dB	Instrument Status :	Used

Calibration Environment and Details

Temperature	: 23 °C ± 2 °C
Humidity	: 50 %RH ± 20 %RH
Barometric Pressure	: 1013 hPa ± 10 hPa
Received Date	: 6 March 2025
Calibrated Date	: 19 March 2025
Calibration Procedure	: In-house method CP-SLM-01 based on IEC 61672-1 : 2013 Electroacoustics - Sound level meters - Part 3: Periodic tests
Location of Calibration	: Lab Acoustic

REVIEW BY ..... Manatsa. P.
APPROVED BY .....
NEXT CAL DATE..... 19/03/26

Reference Standard

Instrument	Brand	Model	SN.	Due calibration	Traceability
Standard Microphone	Brüel & Kjær	4192	2294985	25 June 2025	NIMT
Audio Generator	Svantek	Svan401	131	15 October 2025	WK Electric

Note

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor k = 2, providing a level of confidence approximately 95 %.

Calibrated By : Mr. Noppadon Luangart, Service Calibration Engineer

Approved By : Mr. Pacit Mathavorn, Calibration Engineer Supervisor

Issue Date : 19 March 2025

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd

Certificate No : 25-SLM-114
Request No : Req-2025-0603

1. Indication at the calibration check frequency

UUC Setting	Nominal	Before Adjust		After Adjust		UNCERTAINTY	Acceptance Limit	Result
FAST / A / 30-130	Level	UUC	ERR	UUC	ERR			
Calibrator Setting	(dB)	(dB)	(dB)	(dB)	(dB)	(± dB)	(± dB)	
1000 Hz 94 dB	94.06	94.0	-0.06	94.1	+0.04	0.20	0.30	Pass

Note : Absolute sensitivity was established by the use of Sound Calibrator Brand RION, Model NC-75, SN:35002736

2. Self-generated noise, Microphone installed

UUC Setting	Measured	UNCERTAINTY
FAST / 30-130		
UUC Weighting	(dB)	(± dB)
A	15.4	0.10

3. Self-generated noise, Microphone replaced by the electrical input signal device

UUC Setting	Measured	UNCERTAINTY
FAST / 30-130		
UUC Weighting	(dB)	(± dB)
A	12.2	0.10
C	16.6	0.10
Z	20.4	0.10

4. Acoustic signal test of frequency weightings (Without Windscreen)

UUC Setting	Deviation from various Frequancy Weighting Respone curve			UNCERTAINTY	Acceptance Limit	Result
FAST / 30-130	A	C	Z			
STD Setting	(dB)	(dB)	(dB)	(± dB)	(± dB)	
125 Hz	0.3	0.5	0.5	0.60	1.5	Pass
1000 Hz	0.0	0.0	0.0	0.60	1.0	Pass
4000 Hz	0.4	0.4	0.4	0.60	3.0	Pass
8000 Hz	-1.3	-1.3	-1.3	0.70	5.0	Pass1

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd
FM-708-SLM-01 Rev.04 Issue date 5/6/24

Certificate No : 25-SLM-114
Request No : Req-2025-0603

5. Electrical signal test of frequency weightings, Weighting network respone with relative to 1 kHz

UUC Setting	Deviation from various Frequency Weightine Resnone curve			UNCERTAINTY	Acceptance Limit	Result
FAST / 30-130						
STD Setting	A (dB)	C (dB)	Z (dB)	(± dB)	(± dB)	
63 Hz	-0.1	0.0	0.0	0.20	2.0	Pass
125 Hz	-0.1	0.0	0.0		1.5	Pass
250 Hz	0.0	0.0	0.0		1.5	Pass
500 Hz	0.0	0.1	0.0		1.5	Pass
1000 Hz	0.0	0.0	0.0		1.0	Pass
2000 Hz	0.0	0.1	0.0		2.0	Pass
4000 Hz	0.0	0.0	0.0		3.0	Pass
8000 Hz	0.1	0.1	0.0		5.0	Pass
16000 Hz	-1.3	-1.3	0.0		+5, -INF.	Pass

6. Frequency and time weightings at 1kHz

UUC Setting	STD	Measured		UNCERTAINTY	Acceptance Limit	Result
FAST / 30-130	REF	UUC	ERR			
UUC Weighting	(dB)	(dB)	(dB)	(± dB)	(± dB)	
A	114.00	114.0	0.0	0.20	0.20	Pass
C	114.00	114.0	0.0		0.20	Pass
Z	114.00	114.0	0.0		0.20	Pass

UUC Setting	STD	Measured		UNCERTAINTY	Acceptance Limit	Result
30-130 / A	REF	UUC	ERR			
UUC Time Respone	(dB)	(dB)	(dB)	(± dB)	(± dB)	
Fast	114.00	114.0	0.0	0.20	0.10	Pass1
Slow	114.00	114.0	0.0		0.10	Pass1
Leq	114.00	114.0	0.0		0.10	Pass1

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd
FM-708-SLM-01 Rev.04 Issue date 5/6/24

Certificate No : 25-SLM-114
Request No : Req-2025-0603

7. Long Term Stability

UUC Setting	Measured	UNCERTAINTY	Acceptance Limit	Result
FAST / A / 30-130	UUC			
STD Setting	(dB)	(± dB)	(± dB)	
Initial	114.0	[redacted]		
Final	114.0			
Deviated	0.0	0.10	0.30	Pass

8. Level linearity on the reference level range

UUC Setting	Anticipated	Deviation		UNCERTAINTY	Acceptance Limit	Result
FAST / A / 30-130	REF	UUC	ERR			
STD dB	(dB)	(dB)	(dB)	(± dB)	(± dB)	
138.00	138	137.9	-0.1	0.30	1.1	Pass
134.00	134	134.0	0.0		1.1	Pass
129.00	129	129.0	0.0		1.1	Pass
124.00	124	124.0	0.0		1.1	Pass
119.00	119	119.0	0.0		1.1	Pass
114.00	114	114.0	0.0		1.1	Pass
109.00	109	109.0	0.0		1.1	Pass
104.00	104	104.0	0.0		1.1	Pass
99.00	99	99.0	0.0		1.1	Pass
94.00	94	94.0	0.0		1.1	Pass
89.00	89	89.0	0.0		1.1	Pass
84.00	84	84.0	0.0		1.1	Pass
79.00	79	79.0	0.0		1.1	Pass
74.00	74	74.0	0.0		1.1	Pass
69.00	69	69.0	0.0		1.1	Pass
64.00	64	64.0	0.0		1.1	Pass
59.00	59	59.0	0.0		1.1	Pass
54.00	54	54.0	0.0		1.1	Pass
49.00	49	49.0	0.0		1.1	Pass
44.00	44	44.0	0.0		1.1	Pass
39.00	39	39.0	0.0		1.1	Pass
34.00	34	34.0	0.0		1.1	Pass
29.00	29	29.1	0.1		1.1	Pass
24.00	24	24.0	0.0		1.1	Pass

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd
FM-708-SLM-01 Rev.04 Issue date 5/6/24

Certificate No : 25-SLM-114
Request No : Req-2025-0603

9. Level linearity including the level range control

UUC Setting	STD	Measured		UNCERTAINTY	Acceptance Limit	Result
FAST / A	REF	UUC	ERR			
UUC Range	(dB)	(dB)	(dB)	(± dB)	(± dB)	
30-130	29.50	29.7	0.2	0.30	1.1	Pass
	114	114.0	0.0		1.1	Pass

10. Tone burst response

UUC Setting	STD	Anticipated	Measured		UNCERTAINTY	Acceptance Limit	Result
A / 30-130	Toneburst	Ref	UUC	ERR			
UUC Time Respone	(ms)	(dB)	(dB)	(dB)	(± dB)	(± dB)	
Fast	200	126.0	126.1	+0.1	0.20	1.0	Pass
	2	109.0	109.0	0.0		+1.0, -2.5	Pass
	0.25	100.0	99.9	-0.1		+1.5, -5.0	Pass
Slow	200	119.6	119.6	0.0		1.0	Pass
	2	100.0	100.0	0.0		+1.0, -5.0	Pass
SEL	200	120.0	120.0	0.0		1.0	Pass
	2	100.0	100.0	0.0		+1.0, +2.5	Pass
	0.25	91.0	90.9	-0.1		+1.5, -5.0	Pass

11. Peak C Sound level

UUC Setting	Anticipated	Measured		UNCERTAINTY	Acceptance Limit	Result
FAST / C / 55-141	REF	UUC	ERR			
STD Setting	(dB)	(dB)	(dB)	(± dB)	(± dB)	
Complete cycle	136.4	135.8	-0.60	0.20	3.0	Pass
Positive half cycle	135.4	135.2	-0.20		2.0	Pass
Negative half cycle	135.4	135.2	-0.20		2.0	Pass

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd
FM-708-SLM-01 Rev.04 Issue date 5/6/24

Certificate No : 25-SLM-114
Request No : Req-2025-0603

12. Overload indication

UUC Setting	Measured	UNCERTAINTY	Acceptance Limit	Result
FAST / A / 30-130	UUC			
STD Setting	(dB)	(± dB)	(± dB)	
Positive one-half cycle	139.5	[redacted]		
Negative one-half cycle	139.4			
Deviated	0.1	0.20	1.5	Pass

13. High Level Stability

UUC Setting	Measured	UNCERTAINTY	Acceptance Limit	Result
FAST / A / 30-130	UUC			
STD Setting	(dB)	(± dB)	(± dB)	
Initial	129.0	[redacted]		
Final	129.0			
Deviated	0.0	0.10	0.30	Pass

Note :

Function	Maximum-permitted Uncertainty of measurement
1. Indication at the calibration check frequency	Not applicable
2. Self-generated noise, Microphone installed	Not applicable
3. Self-generated noise, Microphone replaced by the electrical input signal device	Not applicable
4. Acoustic signal test of frequency weightings at 10 Hz to 4 kHz	0.60 dB
4. Acoustic signal test of frequency weightings at >4 kHz to 10 kHz	0.70 dB
5. Electrical signal test of frequency weightings, Weighting network respone with relative to 1 kHz	0.20 dB
6. Frequency and time weightings at 1kHz	0.20 dB
7. Long Term Stability	0.10 dB
8. Level linearity on the reference level range	0.30 dB
9. Level linearity including the level range control	0.30 dB
10. Tone burst response	0.30 dB
11. Peak C Sound level	0.35 dB
12. Overload indication	0.25 dB
13. High Level Stability	0.10 dB

- Acceptance limit and Maximum-permitted Uncertainty was IEC 61672-1:2013

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd
FM-708-SLM-01 Rev.04 Issue date 5/6/24

Certificate No : 25-SLM-114
Request No : Req-2025-0603

Decision Rule for Statements of Conformity


The standard decision rule employed for the statements of conformity to each calibration result will be applied using ILAC-G8:09/2019, Guidelines on the Reporting of Compliance with Specification as following Fig. and statements

Pass = The measurement result plus the expanded uncertainty with a 95% coverage probability were within the limit.

Pass[1] = The measurement result was within the limit. However, a portion of the expanded uncertainty of measurement at 95% exceeds the limit.

Fail[1] = The measurement result was out of the limit. However, a portion of the expanded uncertainty of measurement at 95% is within the limit.

Fail = The measurement result plus the expanded uncertainty with a 95% coverage probability were outside the limit.



End of Certificate

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd
FM-708-SLM-01 Rev.04 Issue date 5/6/24

SITHIPORN ASSOCIATES CO., LTD.
CALIBRATION LABORATORY
481-481/1 Sirinthorn Road, Bangbumru, Bangplad, Bangkok, 10700 Thailand
Tel. +66 2433 8331 Email : calibration@sithiphorn.com

ISO/IEC 17025:2017
CALIBRATION 0394

Cert. No. : ACL25074
Pages : 1 of 8

Calibration Certificate

Equipment : SOUND LEVEL METER
Manufacturer : RION
Model : NL-42 / Microphone UC-52 / Preamplifier NH-24
Serial No.: 00233183 / 157777 / 22653
ID No.: RYG_FS0024

Condition As Found : GOOD

Customer : ALS LABORATORY GROUP (THAILAND) CO., LTD.
104 PHATTHANAKAN 40, PHATTHANAKAN ROAD,
KHWAENG PHATTHANAKAN, KHET SUAN LUANG,
BANGKOK, 10250 THAILAND.

Location : -
Ambient Temperature : (23.0 ± 3) °C
Pressure : (101.3 ± 3) kPa
Relative Humidity : (50.0 ± 20) %

REVIEW BY .....
APPROVED BY .....
NEXT CAL DATE.. 21/ 01/ 2026 .....

Received Date : 07 JANUARY 2025
Calibration Date : 21 - 23 JANUARY 2025
Date of Issue : 24 JANUARY 2025

Calibrated by : Nathakorn Pisutpaisan

Approved by :
(Thanakul Petchurai)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

Cert. No. : ACL25074
Job No. : VC68AC0059
Pages : 2 of 8

Calibration Procedure : CP-AC-01

Calibration Method :
This equipment was calibrated by follow on IEC-61672-3 (2013) Standard for sound level meter (SLM).
The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.
For tests results of each items were made by observation of each Instruments display and also with SLM's display.

Condition of this result of calibration :
1. Reference Standard Instruments :

Instrument	Model	Serial No.	Cert. No.	Due Date
Waveform Generator	33210A	MY48017076	EF-0009-24	05-FEB-25
Waveform Generator	33511B	MY52302742	EF-0007-24	05-FEB-25
Digital Multimeter	34461A	MY53220104	EEL_BP 21/0267	13-FEB-25
Digital Multimeter	34461A	MY53220076	EEL_BP 20/0267	15-FEB-25
Digital Multimeter	34461A	MY60024273	EEL_BP 22/0267	15-FEB-25
Programmable Attenuator	MAT-1070	62100114	EF-0008-24	05-FEB-25
Condenser Microphone	4180	2977900	AA-1001-24	12-FEB-25
Measuring Amplifier	NA-42KAI	34560495	AA-3001-24	05-FEB-25

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.
3. This certificate is traceable to the international system of unit maintained at :
3.1 National Institute of Metrology (Thailand).
3.2 Thailand Institute of Scientific and Technological Research (TISTR).

Cert. No. : ACL25074
Job No. : VC68AC0059
Pages : 3 of 8

Summary of Measurement Result :

Parameter	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	0.2	N/A
2. Self-generated noise	0.2	N/A
3. Acoustical signal tests of frequency weightings		
125 Hz	0.3	0.6
1000 Hz	0.3	0.6
8000 Hz	0.3	0.7
4. Electrical signal tests of frequency weightings		
For 10 Hz to 4 kHz	0.3	0.6
For > 4 kHz to 10 kHz	0.3	0.7
For > 10 kHz to 20 kHz	0.3	1.0
5. Frequency and time weightings at 1 kHz	0.2	0.2
6. Long - term stability	0.1	0.1
7. Level linearity on the reference level range	0.2	0.3
8. Level linearity including the level range control	0.2	0.3
9. Tone burst response	0.2	0.3
10. Peak C sound level	0.2	0.35
11. Overload indication	0.2	0.25
12. High level stability	0.1	0.1

Cert. No. : ACL25074
Job No. : VC68AC0059
Page : 4 of 8

Result of calibration :

1. Absolute sensitivity

Reference Acoustic Signal (dB)	Measured Value (dB)	Deviation (dB)	Acceptance Limit (dB)
93.9 (93.94)	93.9	0.0	±0.3

2. Self-generated noise

2.1 Normal test

Measured Value (dB)
18.2

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Weighting (dB)
A - weight	13.1
C - weight	19.2
Flat	24.9

3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
125	0.7	0.7	0.7	± 1.5
1000	0.0	0.0	0.0	± 1.0
8000	0.0	0.0	0.0	±5.0

Cert. No. : ACL25074
Job No. : VC68AC0059
Pages : 5 of 8

4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	0.0	-0.1	0.0	±2.0
125	0.0	0.0	0.0	±1.5
250	0.0	0.0	0.0	±1.5
500	0.0	0.0	-0.1	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.0	0.0	±2.0
4000	0.0	0.0	0.0	±3.0
8000	0.0	0.1	0.1	±5.0

5. Frequency and time weightings at 1 kHz

5.1 Frequency weightings at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.2
C - weight	94.0	94.0	0.0	± 0.2
Flat	94.0	94.0	0.0	± 0.2

5.2 Time weighting at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	94.0	94.0	0.0	± 0.1
Slow	94.0	94.0	0.0	± 0.1
Leq	94.0	94.0	0.0	± 0.1

6. Long - term stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.3

Cert. No. : ACL25074
Job No. : VC68AC0059
Pages : 6 of 8

7. Level linearity on the reference level range

Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
137.0	137.0	0.0	± 1.1
136.0	136.0	0.0	± 1.1
135.0	135.0	0.0	± 1.1
134.0	134.0	0.0	± 1.1
133.0	132.9	-0.1	± 1.1
132.0	131.9	-0.1	± 1.1
131.0	130.9	-0.1	± 1.1
129.0	129.0	0.0	± 1.1
124.0	124.0	0.0	± 1.1
119.0	119.0	0.0	± 1.1
114.0	114.0	0.0	± 1.1
109.0	109.0	0.0	± 1.1
104.0	104.0	0.0	± 1.1
99.0	99.0	0.0	± 1.1
94.0	94.0	0.0	± 1.1
89.0	89.0	0.0	± 1.1
84.0	84.0	0.0	± 1.1
79.0	79.0	0.0	± 1.1
74.0	74.0	0.0	± 1.1
69.0	69.0	0.0	± 1.1
64.0	64.0	0.0	± 1.1
59.0	59.0	0.0	± 1.1
54.0	54.0	0.0	± 1.1
49.0	49.0	0.0	± 1.1
44.0	44.0	0.0	± 1.1
39.0	39.0	0.0	± 1.1
34.0	34.1	0.1	± 1.1
30.0	30.1	0.1	± 1.1
29.0	29.1	0.1	± 1.1
28.0	28.1	0.1	± 1.1
27.0	27.1	0.1	± 1.1
26.0	26.2	0.2	± 1.1
25.0	25.2	0.2	± 1.1

Cert. No. : ACL25074
Job No. : VC68AC0059
Pages : 7 of 8

8. Level linearity including the level range control

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
130	94.0	94.0	0.0	±1.1

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
130	29.0	29.1	0.1	±1.1

9. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Cycle	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.0	0.0	±1.0
Slow	2	8	108.0	108.0	0.0	1.5 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
SEL	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.0	0.0	±1.0

Cert. No. : ACL25074
Job No. : VC68AC0059
Pages : 8 of 8

10. Peak C sound level

Number of cycle in test signal	Anticipated Value (dB)	Measured Value, Lcpeak (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	130.0	130.0	0.0	±3.0
One	133.4	133.4	0.0	±3.0

Number of cycle in test signal	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	±2.0
Positive half cycle	135.4	135.2	-0.2	±2.0
Negative half cycle	135.4	135.2	-0.2	±2.0

11. Overload indication

Measured value (dB)		Deviated Value (dB)	Acceptance Limits (dB)
Positive one-half cycle	Negative one-half cycle		
89.5	89.5	0.0	±1.5

12. High level stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor $k = 2$ or any value following calculation,providing a level of confidence of approximately 95 %

End of Calibration Certificate

SITHIPORN ASSOCIATES CO., LTD.
CALIBRATION LABORATORY
45/1-45/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand
Tel. +66 2433 8331 Email : calibration@sithiphorn.com

Cert. No. : ACL25075
Pages : 1 of 8

Calibration Certificate

Equipment :	SOUND LEVEL METER
Manufacturer :	RION
Model :	NL-42 / Microphone UC-52 / Preamplifier NH-24
Serial No.:	00233184 / 144837 / 23232
ID No.:	RYG_FS0025
Condition As Found :	GOOD
Customer :	ALS LABORATORY GROUP (THAILAND) CO., LTD. 104 PHATTHANAKAN 40, PHATTHANAKAN ROAD, KHWAENG PHATTHANAKAN, KHET SUAN LUANG, BANGKOK, 10250 THAILAND.
Location :	-
Ambient Temperature :	(23.0 ± 3) °C
Pressure :	(101.3 ± 3) kPa
Relative Humidity :	(50.0 ± 20) %
Received Date :	07 JANUARY 2025
Calibration Date :	21 - 23 JANUARY 2025
Date of Issue :	24 JANUARY 2025

REVIEW BY .....
APPROVED BY.....
NEXT CAL DATE..... 21 /01 /2026

Calibrated by : Nathakorn Pisutpaisan

Approved by : (Thanakul Petchurai)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

Cert. No. : ACL25075
Job No. : VC68AC0059
Pages : 2 of 8

Calibration Procedure : CP-AC-01

Calibration Method :

This equipment was calibrated by follow on IEC-61672-3 (2013) Standard for sound level meter (SLM).
The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.
For tests results of each items were made by observation of each Instruments display and also with SLM's display.

Condition of this result of calibration :

1. Reference Standard Instruments :

Instrument	Model	Serial No.	Cert. No.	Due Date
Waveform Generator	33210A	MY48017076	EF-0009-24	05-FEB-25
Waveform Generator	33511B	MY52302742	EF-0007-24	05-FEB-25
Digital Multimeter	34461A	MY53220104	EEL_BP 21/0267	13-FEB-25
Digital Multimeter	34461A	MY53220076	EEL_BP 20/0267	15-FEB-25
Digital Multimeter	34461A	MY60024273	EEL_BP 22/0267	15-FEB-25
Programmable Attenuator	MAT-1070	62100114	EF-0008-24	05-FEB-25
Condenser Microphone	4180	2977900	AA-1001-24	12-FEB-25
Measuring Amplifier	NA-42KAI	34560495	AA-3001-24	05-FEB-25

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.
3. This certificate is traceable to the international system of unit maintained at :
   3.1 National Institute of Metrology (Thailand).
   3.2 Thailand Institute of Scientific and Technological Research (TISTR).

Cert. No. : ACL25075
Job No. : VC68AC0059
Pages : 3 of 8

Summary of Measurement Result :

Parameter	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	0.2	N/A
2. Self-generated noise	0.2	N/A
3. Acoustical signal tests of frequency weightings		
125 Hz	0.3	0.6
1000 Hz	0.3	0.6
8000 Hz	0.3	0.7
4. Electrical signal tests of frequency weightings		
For 10 Hz to 4 kHz	0.3	0.6
For > 4 kHz to 10 kHz	0.3	0.7
For > 10 kHz to 20 kHz	0.3	1.0
5. Frequency and time weightings at 1 kHz	0.2	0.2
6. Long - term stability	0.1	0.1
7. Level linearity on the reference level range	0.2	0.3
8. Level linearity including the level range control	0.2	0.3
9. Tone burst response	0.2	0.3
10. Peak C sound level	0.2	0.35
11. Overload indication	0.2	0.25
12. High level stability	0.1	0.1

Cert. No. : ACL25075
Job No. : VC68AC0059
Page : 4 of 8

Result of calibration :

1. Absolute sensitivity

Reference Acoustic Signal (dB)	Measured Value (dB)	Deviation (dB)	Acceptance Limit (dB)
93.9 (93.94)	93.9	0.0	±0.3

2. Self-generated noise

2.1 Normal test

Measured Value (dB)
18.2

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Weighting (dB)
A - weight	11.6
C - weight	17.8
Flat	23.5

3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
125	0.4	0.4	0.4	± 1.5
1000	0.0	0.0	0.0	± 1.0
8000	-0.4	-0.4	-0.4	±5.0

Cert. No. : ACL25075
Job No. : VC68AC0059
Pages : 5 of 8

4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	0.0	0.0	0.0	±2.0
125	0.0	0.1	0.0	±1.5
250	0.0	0.0	0.0	±1.5
500	0.0	0.1	0.0	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.1	0.0	±2.0
4000	0.0	0.0	0.0	±3.0
8000	0.0	0.1	0.1	±5.0

5. Frequency and time weightings at 1 kHz

5.1 Frequency weightings at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.2
C - weight	94.0	94.0	0.0	± 0.2
Flat	94.0	94.0	0.0	± 0.2

5.2 Time weighting at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	94.0	94.0	0.0	± 0.1
Slow	94.0	94.0	0.0	± 0.1
Leq	94.0	94.0	0.0	± 0.1

6. Long - term stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.3

T. Petchu.

Cert. No. : ACL25075
Job No. : VC68AC0059
Pages : 6 of 8

7. Level linearity on the reference level range

Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
137.0	137.0	0.0	± 1.1
136.0	136.0	0.0	± 1.1
135.0	135.0	0.0	± 1.1
134.0	134.0	0.0	± 1.1
133.0	133.0	0.0	± 1.1
132.0	132.0	0.0	± 1.1
131.0	131.0	0.0	± 1.1
129.0	129.0	0.0	± 1.1
124.0	124.0	0.0	± 1.1
119.0	119.0	0.0	± 1.1
114.0	114.0	0.0	± 1.1
109.0	109.0	0.0	± 1.1
104.0	104.0	0.0	± 1.1
99.0	99.0	0.0	± 1.1
94.0	94.0	0.0	± 1.1
89.0	89.0	0.0	± 1.1
84.0	84.0	0.0	± 1.1
79.0	79.0	0.0	± 1.1
74.0	74.0	0.0	± 1.1
69.0	69.0	0.0	± 1.1
64.0	64.0	0.0	± 1.1
59.0	59.0	0.0	± 1.1
54.0	54.0	0.0	± 1.1
49.0	49.0	0.0	± 1.1
44.0	44.0	0.0	± 1.1
39.0	39.0	0.0	± 1.1
34.0	34.0	0.0	± 1.1
30.0	30.0	0.0	± 1.1
29.0	29.0	0.0	± 1.1
28.0	28.0	0.0	± 1.1
27.0	27.1	0.1	± 1.1
26.0	26.0	0.0	± 1.1
25.0	25.1	0.1	± 1.1

T. Petchu.

Cert. No. : ACL25075
Job No. : VC68AC0059
Pages : 7 of 8

8. Level linearity including the level range control

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
130	94.0	94.0	0.0	±1.1

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
130	29.0	29.0	0.0	±1.1

9. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Cycle	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.1	0.1	±1.0
Slow	2	8	108.0	108.0	0.0	1.5 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
SEL	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.1	0.1	±1.0

T. Petchu.

Cert. No. : ACL25075
Job No. : VC68AC0059
Pages : 8 of 8

10. Peak C sound level

Number of cycle in test signal	Anticipated Value (dB)	Measured Value, Lcpeak (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	130.0	130.0	0.0	±3.0
One	133.4	133.4	0.0	±3.0

Number of cycle in test signal	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	±2.0
Positive half cycle	135.4	135.2	-0.2	±2.0
Negative half cycle	135.4	135.2	-0.2	±2.0

11. Overload indication

Measured value (dB)		Deviated Value (dB)	Acceptance Limits (dB)
Positive one-half cycle	Negative one-half cycle		
89.6	89.5	-0.1	±1.5

12. High level stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor $k = 2$ or any value following calculation,providing a lavel of confidence of approximately 95 %

End of Calibration Certificate

T. Petchu.

SITHIPORN ASSOCIATES CO., LTD.
CALIBRATION LABORATORY
493~493/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand
Tel. +66 2433 8331 Email : calibration@sithiporn.com

Cert. No. : ACL25079
Page : 1 of 8

Calibration Certificate

Equipment : SOUND LEVEL METER
Manufacturer : RION
Model : NL-42A/ Microphone UC-52 / Preamplifier NH-24
Serial No.: 00623394 / 198641 / 26422
ID No.: RYG_FS0619

Condition As Found : GOOD

Customer : ALS LABORATORY GROUP (THAILAND) CO., LTD.
104 PHATTHANAKAN 40, PHATTHANAKAN ROAD,
KHWAENG PHATTHANAKAN, KHET SUAN LUANG,
BANGKOK, 10250 THAILAND.

Location : -
Ambient Temperature : (23.0 ± 3) °C
Pressure : (101.3 ± 3) kPa
Relative Humidity : (50.0 ± 20) %

Received Date : 07 JANUARY 2025
Calibration Date : 21 - 23 JANUARY 2025
Date of Issue : 24 JANUARY 2025

REVIEW BY .....
APPROVED BY .....
NEXT CAL DATE..... 21/ 01/ 2026

Calibrated by : Nathakorn Pisutpaisan

Approved by :
T. Petchu.
(Thanakul Petchurai)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

Cert. No. : ACL25079
Job No. : VC68AC0059
Pages : 2 of 8

Calibration Procedure : CP-AC-01

Calibration Method :

This equipment was calibrated by follow on IEC-61672-3 (2013) Standard for sound level meter (SLM).
The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.
For tests results of each items were made by observation of each Instruments display and also with SLM's display.

Condition of this result of calibration :

1. Reference Standard Instruments :

Instrument	Model	Serial No.	Cert. No.	Due Date
Waveform Generator	33210A	MY48017076	EF-0009-24	05-FEB-25
Waveform Generator	33511B	MY52302742	EF-0007-24	05-FEB-25
Digital Multimeter	33461A	MY53220104	EEL.BP 21/0267	13-FEB-25
Digital Multimeter	33461A	MY53220076	EEL.BP 20/0267	15-FEB-25
Digital Multimeter	34461A	MY60024273	EEL.BP 22/0267	15-FEB-25
Programmable Attenuator	MAT-1070	62100114	EF-0008-24	05-FEB-25
Condenser Microphone	4180	2977900	AA-1001-24	12-FEB-25
Measuring Amplifier	NA-42KAI	34560495	AA-3001-24	05-FEB-25

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.
3. This certificate is traceable to the international system of unit maintained at :
   3.1 National Institute of Metrology (Thailand).
   3.2 Thailand Institute of Scientific and Technological Research (TISTR).

T. Petchu.

Cert. No. : ACL25079
Job No. : VC68AC0059
Pages : 3 of 8

Summary of Measurement Result :

Parameter	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	0.2	N/A
2. Self-generated noise	0.2	N/A
3. Acoustical signal tests of frequency weightings		
125 Hz	0.3	0.6
1000 Hz	0.3	0.6
8000 Hz	0.3	0.7
4. Electrical signal tests of frequency weightings		
For 10 Hz to 4 kHz	0.3	0.6
For > 4 kHz to 10 kHz	0.3	0.7
For > 10 kHz to 20 kHz	0.3	1.0
5. Frequency and time weightings at 1 kHz	0.2	0.2
6. Long - term stability	0.1	0.1
7. Level linearity on the reference level range	0.2	0.3
8. Level linearity including the level range control	0.2	0.3
9. Tone burst response	0.2	0.3
10. Peak C sound level	0.2	0.35
11. Overload indication	0.2	0.25
12. High level stability	0.1	0.1

T. Petchu.

Cert. No. : ACL25079
Job No. : VC68AC0059
Page : 4 of 8

Result of calibration :

1. Absolute sensitivity

Reference Acoustic Signal (dB)	Measured Value (dB)	Deviation (dB)	Acceptance Limit (dB)
93.9 (93.94)	93.9	0.0	±0.3

2. Self-generated noise

2.1 Normal test

Measured Value (dB)
14.6

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Weighting (dB)
A - weight	12.6
C - weight	19.1
Flat	24.5

3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
125	0.4	0.4	0.4	± 1.5
1000	0.1	0.1	0.1	± 1.0
8000	0.1	0.1	0.1	±5.0

T. Petchu.

Cert. No. : ACL25079
Job No. : VC68AC0059
Pages : 5 of 8

4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	0.0	-0.1	0.0	±2.0
125	0.0	0.0	0.0	±1.5
250	0.0	0.0	0.0	±1.5
500	0.0	0.0	0.0	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.0	0.0	±2.0
4000	0.0	0.0	0.0	±3.0
8000	0.0	0.1	0.1	±5.0

5. Frequency and time weightings at 1 kHz

5.1 Frequency weightings at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.2
C - weight	94.0	94.0	0.0	± 0.2
Flat	94.0	94.0	0.0	± 0.2

5.2 Time weighting at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	94.0	94.0	0.0	± 0.1
Slow	94.0	94.0	0.0	± 0.1
Leq	94.0	94.0	0.0	± 0.1

6. Long - term stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.3

T. Petchu.

Cert. No. : ACL25079
Job No. : VC68AC0059
Pages : 6 of 8

7. Level linearity on the reference level range

Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
137.0	137.0	0.0	± 1.1
136.0	136.0	0.0	± 1.1
135.0	135.0	0.0	± 1.1
134.0	134.0	0.0	± 1.1
133.0	133.0	0.0	± 1.1
132.0	132.0	0.0	± 1.1
131.0	131.0	0.0	± 1.1
129.0	129.0	0.0	± 1.1
124.0	124.0	0.0	± 1.1
119.0	119.0	0.0	± 1.1
114.0	114.0	0.0	± 1.1
109.0	109.0	0.0	± 1.1
104.0	104.0	0.0	± 1.1
99.0	99.0	0.0	± 1.1
94.0	94.0	0.0	± 1.1
89.0	89.0	0.0	± 1.1
84.0	84.0	0.0	± 1.1
79.0	79.0	0.0	± 1.1
74.0	74.0	0.0	± 1.1
69.0	69.0	0.0	± 1.1
64.0	64.0	0.0	± 1.1
59.0	59.0	0.0	± 1.1
54.0	54.0	0.0	± 1.1
49.0	49.0	0.0	± 1.1
44.0	44.0	0.0	± 1.1
39.0	39.0	0.0	± 1.1
34.0	34.1	0.1	± 1.1
30.0	30.1	0.1	± 1.1
29.0	29.1	0.1	± 1.1
28.0	28.1	0.1	± 1.1
27.0	27.1	0.1	± 1.1
26.0	26.1	0.1	± 1.1
25.0	25.1	0.1	± 1.1

Cert. No. : ACL25079
Job No. : VC68AC0059
Pages : 7 of 8

8. Level linearity including the level range control

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
130	94.0	94.0	0.0	±1.1

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
130	29.0	28.9	-0.1	±1.1

9. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Cycle	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.0	0.0	±1.0
Slow	2	8	108.0	108.0	0.0	1.5 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
SEL	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	120.0	120.0	0.0	±1.0

Cert. No. : ACL25079
Job No. : VC68AC0059
Pages : 8 of 8

10. Peak C sound level

Number of cycle in test signal	Anticipated Value (dB)	Measured Value, Lcpeak (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	130.0	130.0	0.0	±3.0
One	133.4	133.3	-0.1	±3.0

Number of cycle in test signal	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	132.9	-0.1	±2.0
Positive half cycle	135.4	135.1	-0.3	±2.0
Negative half cycle	135.4	135.1	-0.3	±2.0

11. Overload indication

Measured value (dB)		Deviated Value (dB)	Acceptance Limits (dB)
Positive one-half cycle	Negative one-half cycle		
89.5	89.6	0.1	±1.5

12. High level stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	113.0	113.0	0.0	±0.5

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor $k = 2$ or any value following calculation,providing a lavel of confidence of approximately 95 %

End of Calibration Certificate

Certificate of Calibration

Customer

Name : ALS Laboratory Group Thailand Co., Ltd.
Address : 104 Soi Phatthanakan 40, Phatthanakan Road, Suan Luang, Bangkok 10250

Certificate No : 25-ACT-042
Request No : Req-2025-0604

Unit Under Calibration Details

Measurement item : Acoustic Calibrator
Manufacturer : RION
Model : NC-75
Serial Number : 35002736
ID : RYG_FS0496

Class : 1
Range : 94 dB / 1000 Hz
Instrument Status : Used

Calibration Environment and Details

Tempenture : (23 ±2 °C)
Humidity : (50 ± 20 %RH)
Barometric Pressure : (1013 ±10.0 hPa)
Received Date : 6 March 2025
Calibration Date : 19 March 2025
Location of Calibration : LAB 1 Acoustic
Calibration Procedure : In-house method CP-ACT-02 based on IEC 60942:2017 Electroacoustics - Sound calibrators

REVIEW BY .....
APPROVED BY .....
NEXT CAL DATE 19/03/26

Reference Standard	Model	Serial Number	Traceable	Due Calibration
Sound Calibrator	SV 35A	58079	EEI	12 June 2025
THD Multimeter	2015	1647765	NIMT	4 February 2026

Traceability : This certificate providoes traceability of measurement to recognized national standard, and to the realization of the international System of Units (SI).

Note

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor k =2, providing a level of confidence approximately 95 %.

Calibrated By : Mr. Noppadon Luangart, Service Calibration Engineer

Approved By : Mr. Pacit Mathavorn, Calibration Engineer Supervisor

Issue Date : 19 March 2025

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.
FM-708-ACT-02 Rev.03 Issue date 5/6/24

Certificate No : 25-ACT-042
Request No : Req-2025-0604

Sound pressure level — **Calibration Results :** Without Adjustment

Calibration Range (dB)	Without Adjustment (dB)		Adjustment (dB)		Uncertainty (± dB)	Acceptance limit Class 1 (± dB)	Result
	Measured	Deviated value	Measured	Deviated value			
94 dB / 1000 Hz	94.06	0.06	-	-	0.13	0.25	Pass

Frequency of Sound pressure level

Calibration Range (Hz)	Without Adjustment		Adjustment		Uncertainty (± %)	Acceptance limit Class 1 (± %)	Result
	Measured (Hz)	Deviated	Measured (Hz)	Deviated			
94 dB / 1000 Hz	1000.00	0.00	-	-	0.01	0.70	Pass

Total Harmonic Distortion plus Noise of Sound pressure level(THD+N %)

Calibration Range (Hz)	Without Adjustment	Adjustment	Uncertainty (± %)	Acceptance limit Class 1 (± %)	Result
	Measured (%)	Measured (%)			
94 dB / 1000 Hz	0.98	-	0.40	2.5	Pass

Note :

Function	Maximum-permitted Uncertainty of measurement
Sound pressure level	0.15 dB
Frequency	0.20%
Total distortion+noise	0.50%

* Acceptance limit was IEC60942:2017 Class 1
- The calibration results exclude the calibrator pressure correction
- The calibration results exclude the microphone volume correction

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.
FM-708-ACT-02 Rev.03 Issue date 5/6/24

Certificate No : 25-ACT-042
Request No : Req-2025-0604

Decision Rule for Statements of Conformity


The standard decision rule employed for the statements of conformity to each calibration result will be applied using ILAC-G8:09/2019, Guidelines on the Reporting of Compliance with Specification as following Fig. and statements

Pass = The measurement result plus the expanded uncertainty with a 95% coverage probability were within the limit.

Pass' = The measurement result was within the limit. However, a portion of the expanded uncertainty of measurement at 95% exceeds the limit.

Fail' = The measurement result was out of the limit. However, a portion of the expandeduncertainty of measurement at 95% is within the limit.

Fail = The measurement result plus the expanded uncertainty with a 95% coverage probability were outside the limit.



End of Calibration

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.
FM-708-ACT-02 Rev.03 Issue date 5/6/24

SITHIPORN ASSOCIATES CO., LTD.
CALIBRATION LABORATORY
451-451/1 Sirinthorn Road, Bangbumru, Bangplad, Bangkok, 10700 Thailand
Tel. +66 2433 8331 Email : calibration@sithiphorn.com

Cert. No. : ACL25079
Pages : 1 of 8

Calibration Certificate

Equipment : SOUND LEVEL METER
Manufacturer : RION
Model : NL-42A/ Microphone UC-52 / Preamplifier NH-24
Serial No.: 00623394 / 198641 / 26422
ID No.: RYG_FS0619

Condition As Found : GOOD

Customer : ALS LABORATORY GROUP (THAILAND) CO., LTD.
104 PHATTHANAKAN 40, PHATTHANAKAN ROAD,
KHWAENG PHATTHANAKAN, KHET SUAN LUANG,
BANGKOK, 10250 THAILAND.

Location : -
Ambient Temperature : (23.0 ± 3) °C
Pressure : (101.3 ± 3) kPa
Relative Humidity : (50.0 ± 20) %

Received Date : 07 JANUARY 2025
Calibration Date : 21 - 23 JANUARY 2025
Date of Issue : 24 JANUARY 2025

REVIEW BY .....
APPROVED BY .....
NEXT CAL DATE 21/ 01/ 2026

Calibrated by : Nathakorn Pisutpaisan

Approved by : (Thanakul Petchurai)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

Cert. No. : ACL25079
Job No. : VC68AC0059
Pages : 2 of 8

Calibration Procedure : CP-AC-01

Calibration Method :

This equipment was calibrated by follow on IEC-61672-3 (2013) Standard for sound level meter (SLM).
The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.
For tests results of each items were made by observation of each Instruments display and also with SLM's display.

Condition of this result of calibration :

1. Reference Standard Instruments :

Instrument	Model	Serial No.	Cert. No.	Due Date
Waveform Generator	33210A	MY48017076	EF-0009-24	05-FEB-25
Waveform Generator	33511B	MY52302742	EF-0007-24	05-FEB-25
Digital Multimeter	33461A	MY53220104	EEL.BP 21/0267	13-FEB-25
Digital Multimeter	33461A	MY53220076	EEL.BP 20/0267	15-FEB-25
Digital Multimeter	34461A	MY60024273	EEL.BP 22/0267	15-FEB-25
Programmable Attenuator	MAT-1070	62100114	EF-0008-24	05-FEB-25
Condenser Microphone	4180	2977900	AA-1001-24	12-FEB-25
Measuring Amplifier	NA-42KAI	34560495	AA-3001-24	05-FEB-25

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.
3. This certificate is traceable to the international system of unit maintained at :
   3.1 National Institute of Metrology (Thailand).
   3.2 Thailand Institute of Scientific and Technological Research (TISTR).

FM-708-ACT-02 Rev.03 Issue date 5/6/24

Cert. No. : ACL25079
Job No. : VC68AC0059
Pages : 3 of 8

Summary of Measurement Result :

Parameter	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	0.2	N/A
2. Self-generated noise	0.2	N/A
3. Acoustical signal tests of frequency weightings		
125 Hz	0.3	0.6
1000 Hz	0.3	0.6
8000 Hz	0.3	0.7
4. Electrical signal tests of frequency weightings		
For 10 Hz to 4 kHz	0.3	0.6
For > 4 kHz to 10 kHz	0.3	0.7
For > 10 kHz to 20 kHz	0.3	1.0
5. Frequency and time weightings at 1 kHz	0.2	0.2
6. Long - term stability	0.1	0.1
7. Level linearity on the reference level range	0.2	0.3
8. Level linearity including the level range control	0.2	0.3
9. Tone burst response	0.2	0.3
10. Peak C sound level	0.2	0.35
11. Overload indication	0.2	0.25
12. High level stability	0.1	0.1

FM-708-ACT-02 Rev.03 Issue date 5/6/24

Cert. No. : ACL25079
Job No. : VC68AC0059
Page : 4 of 8

Result of calibration :

1. Absolute sensitivity

Reference Acoustic Signal (dB)	Measured Value (dB)	Deviation (dB)	Acceptance Limit (dB)
93.9 (93.94)	93.9	0.0	±0.3

2. Self-generated noise

2.1 Normal test

Measured Value (dB)
14.6

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Weighting (dB)
A - weight	12.6
C - weight	19.1
Flat	24.5

3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
125	0.4	0.4	0.4	± 1.5
1000	0.1	0.1	0.1	± 1.0
8000	0.1	0.1	0.1	±5.0

Cert. No. : ACL25079
Job No. : VC68AC0059
Pages : 5 of 8

4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	0.0	-0.1	0.0	±2.0
125	0.0	0.0	0.0	±1.5
250	0.0	0.0	0.0	±1.5
500	0.0	0.0	0.0	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.0	0.0	±2.0
4000	0.0	0.0	0.0	±3.0
8000	0.0	0.1	0.1	±5.0

5. Frequency and time weightings at 1 kHz

5.1 Frequency weightings at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.2
C - weight	94.0	94.0	0.0	± 0.2
Flat	94.0	94.0	0.0	± 0.2

5.2 Time weighting at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	94.0	94.0	0.0	± 0.1
Slow	94.0	94.0	0.0	± 0.1
Leq	94.0	94.0	0.0	± 0.1

6. Long - term stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.3

Cert. No. : ACL25079
Job No. : VC68AC0059
Pages : 6 of 8

7. Level linearity on the reference level range

Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
137.0	137.0	0.0	± 1.1
136.0	136.0	0.0	± 1.1
135.0	135.0	0.0	± 1.1
134.0	134.0	0.0	± 1.1
133.0	133.0	0.0	± 1.1
132.0	132.0	0.0	± 1.1
131.0	131.0	0.0	± 1.1
129.0	129.0	0.0	± 1.1
124.0	124.0	0.0	± 1.1
119.0	119.0	0.0	± 1.1
114.0	114.0	0.0	± 1.1
109.0	109.0	0.0	± 1.1
104.0	104.0	0.0	± 1.1
99.0	99.0	0.0	± 1.1
94.0	94.0	0.0	± 1.1
89.0	89.0	0.0	± 1.1
84.0	84.0	0.0	± 1.1
79.0	79.0	0.0	± 1.1
74.0	74.0	0.0	± 1.1
69.0	69.0	0.0	± 1.1
64.0	64.0	0.0	± 1.1
59.0	59.0	0.0	± 1.1
54.0	54.0	0.0	± 1.1
49.0	49.0	0.0	± 1.1
44.0	44.0	0.0	± 1.1
39.0	39.0	0.0	± 1.1
34.0	34.1	0.1	± 1.1
30.0	30.1	0.1	± 1.1
29.0	29.1	0.1	± 1.1
28.0	28.1	0.1	± 1.1
27.0	27.1	0.1	± 1.1
26.0	26.1	0.1	± 1.1
25.0	25.1	0.1	± 1.1

Cert. No. : ACL25079
Job No. : VC68AC0059
Pages : 7 of 8

8. Level linearity including the level range control

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
130	94.0	94.0	0.0	±1.1

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
130	29.0	28.9	-0.1	±1.1

9. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Cycle	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.0	0.0	±1.0
Slow	2	8	108.0	108.0	0.0	1.5 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
SEL	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.0	0.0	±1.0

Cert. No. : ACL25079
Job No. : VC68AC0059
Pages : 8 of 8

10. Peak C sound level

Number of cycle in test signal	Anticipated Value (dB)	Measured Value, Lcpeak (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	130.0	130.0	0.0	±3.0
One	133.4	133.3	-0.1	±3.0

Number of cycle in test signal	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	132.9	-0.1	±2.0
Positive half cycle	135.4	135.1	-0.3	±2.0
Negative half cycle	135.4	135.1	-0.3	±2.0

11. Overload indication

Measured value (dB)		Deviated Value (dB)	Acceptance Limits (dB)
Positive one-half cycle	Negative one-half cycle		
89.5	89.6	0.1	±1.5

12. High level stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor $k = 2$ or any value following calculation,providing a lavel of confidence of approximately 95 %

End of Calibration Certificate

SITHIPORN ASSOCIATES CO., LTD.
CALIBRATION LABORATORY
451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand
Tel. +66 2433 8331 Email : calibration@sithiphorn.com

Cert. No. : ACL25112
Pages : 1 of 8

Calibration Certificate

Equipment : SOUND LEVEL METER
Manufacturer : RION
Model : NL-42A / Microphone UC-52 / Preamplifier NH-24
Serial No.: 00623396 / 198643 / 26424
ID No.: RYG_FS0621

Condition As Found : GOOD

Customer : ALS LABORATORY GROUP (THAILAND) CO., LTD.
104 PHATTHANAKAN 40, PHATTHANAKAN ROAD,
KHWAENG PHATTHANAKAN, KHET SUAN LUANG,
BANGKOK, 10250 THAILAND.

Location : -
Ambient Temperature : (23.0 ± 3) °C
Pressure : (101.3 ± 3) kPa
Relative Humidity : (50.0 ± 20) %

REVIEW BY
APPROVED BY
NEXT CAL DATE. 26/ 01/ 2026

Received Date : 14 JANUARY 2025
Calibration Date : 27-29 JANUARY 2025
Date of Issue : 30 JANUARY 2025

Calibrated by : Nathakorn Pisutpaisan

Approved by : (Thanakul Petchurai)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

Cert. No. : ACL25112
Job No. : VC68AC0064
Pages : 2 of 8

Calibration Procedure : CP-AC-01

Calibration Method :

This equipment was calibrated by follow on IEC-61672-3 (2013) Standard for sound level meter (SLM).
The SLM had tests to Acoustical and Electrical signal tests cf frequency weighting with Anechoic chamber and Reference Standard Instruments.
For tests results of each items were made by observation of each Instruments display and also with SLM's display.

Condition of this result of calibration :

1. Reference Standard Instruments :

Instrument	Model	Serial No.	Cert. No.	Due Date
Waveform Generator	33210A	MY48017076	EF-0009-24	05-FEB-25
Waveform Generator	33511B	MY53202742	EF-0007-24	05-FEB-25
Digital Multimeter	34461A	MY53220104	EEL_BP 21/0267	13-FEB-25
Digital Multimeter	34461A	MY53220076	EEL_BP 20/0267	13-FEB-25
Digital Multimeter	34461A	MY60024273	EEL_BP 22/0267	15-FEB-25
Programmable Attenuator	MAT-1070	62100114	EF-0008-24	05-FEB-25
Condenser Microphone	4180	2977900	AA-1001-24	12-FEB-25
Measuring Amplifier	NA-42KAI	34560495	AA-3001-24	05-FEB-25

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.
3. This certificate is traceable to the international system of unit maintained at :
   3.1 National Institute of Metrology (Thailand).
   3.2 Thailand Institute of Scientific and Technological Research (TISTR).

Cert. No. : ACL25112
Job No. : VC68AC0064
Pages : 3 of 8

Summary of Measurement Result :

Parameter	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	0.2	N/A
2. Self-generated noise	0.2	N/A
3. Acoustical signal tests of frequency weightings		
125 Hz	0.3	0.6
1000 Hz	0.3	0.6
8000 Hz	0.3	0.7
4. Electrical signal tests of frequency weightings		
For 10 Hz to 4 kHz	0.3	0.6
For > 4 kHz to 10 kHz	0.3	0.7
For > 10 kHz to 20 kHz	0.3	1.0
5. Frequency and time weightings at 1 kHz	0.2	0.2
6. Long - term stability	0.1	0.1
7. Level linearity on the reference level range	0.2	0.3
8. Level linearity including the level range control	0.2	0.3
9. Tone burst response	0.2	0.3
10. Peak C sound level	0.2	0.35
11. Overload indication	0.2	0.25
12. High level stability	0.1	0.1

Cert. No. : ACL25112
Job No. : VC68AC0064
Page : 4 of 8

Result of calibration :

1. Absolute sensitivity

Reference Acoustic Signal (dB)	Measured Value (dB)	Deviation (dB)	Acceptance Limit (dB)
93.9 (93.94)	93.9	0.0	±0.3

2. Self-generated noise

2.1 Normal test

Measured Value (dB)
14.8

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Weighting (dB)
A - weight	11.3
C - weight	18.9
Flat	24.4

3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
125	0.3	0.3	0.3	± 1.5
1000	0.1	0.1	0.1	± 1.0
8000	0.6	0.6	0.6	±5.0

Cert. No. : ACL25112
Job No. : VC68AC0064
Pages : 5 of 8

4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	0.0	0.1	0.1	±2.0
125	0.1	0.1	0.1	±1.5
250	0.1	0.1	0.0	±1.5
500	0.0	0.1	0.0	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.1	0.0	±2.0
4000	0.0	0.0	0.0	±3.0
8000	0.0	0.1	0.1	±5.0

5. Frequency and time weightings at 1 kHz

5.1 Frequency weightings at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.2
C - weight	94.0	94.0	0.0	± 0.2
Flat	94.0	94.0	0.0	± 0.2

5.2 Time weighting at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	94.0	94.0	0.0	± 0.1
Slow	94.0	94.0	0.0	± 0.1
Leq	94.0	94.0	0.0	± 0.1

6. Long - term stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.1	0.1	± 0.3

T. Retchn.

Cert. No. : ACL25112
Job No. : VC68AC0064
Pages : 6 of 8

7. Level linearity on the reference level range

Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
137.0	137.0	0.0	± 1.1
136.0	136.0	0.0	± 1.1
135.0	135.0	0.0	± 1.1
134.0	134.0	0.0	± 1.1
133.0	133.0	0.0	± 1.1
132.0	132.0	0.0	± 1.1
131.0	131.0	0.0	± 1.1
129.0	129.0	0.0	± 1.1
124.0	124.0	0.0	± 1.1
119.0	119.0	0.0	± 1.1
114.0	114.0	0.0	± 1.1
109.0	109.0	0.0	± 1.1
104.0	104.0	0.0	± 1.1
99.0	99.0	0.0	± 1.1
94.0	94.0	0.0	± 1.1
89.0	89.0	0.0	± 1.1
84.0	84.0	0.0	± 1.1
79.0	79.0	0.0	± 1.1
74.0	74.0	0.0	± 1.1
69.0	69.0	0.0	± 1.1
64.0	64.0	0.0	± 1.1
59.0	59.0	0.0	± 1.1
54.0	54.0	0.0	± 1.1
49.0	49.0	0.0	± 1.1
44.0	44.0	0.0	± 1.1
39.0	39.0	0.0	± 1.1
34.0	34.0	0.0	± 1.1
30.0	30.1	0.1	± 1.1
29.0	29.0	0.0	± 1.1
28.0	28.1	0.1	± 1.1
27.0	27.1	0.1	± 1.1
26.0	26.2	0.2	± 1.1
25.0	25.1	0.1	± 1.1

T. Retchn.

Cert. No. : ACL25112
Job No. : VC68AC0064
Pages : 7 of 8

8. Level linearity including the level range control

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
130	94.0	94.0	0.0	±1.1

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
130	29.0	29.1	0.1	±1.1

9. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Cycle	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.1	0.1	±1.0
Slow	2	8	108.0	108.0	0.0	1.5 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
SEL	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.1	0.1	±1.0

T. Retchn.

Cert. No. : ACL25112
Job No. : VC68AC0064
Pages : 8 of 8

10. Peak C sound level

Number of cycle in test signal	Anticipated Value (dB)	Measured Value, Lcpeak (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	130.0	130.0	0.0	±3.0
One	133.4	133.4	0.0	±3.0

Number of cycle in test signal	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	±2.0
Positive half cycle	135.4	135.1	-0.3	±2.0
Negative half cycle	135.4	135.1	-0.3	±2.0

11. Overload indication

Measured value (dB)		Deviated Value (dB)	Acceptance Limits (dB)
Positive one-half cycle	Negative one-half cycle		
89.6	89.6	0.0	±1.5

12. High level stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor $k = 2$ or any value following calculation,providing a level of confidence of approximately 95 %

End of Calibration Certificate

T. Retchn.

CERTIFICATE OF CALIBRATION

ISSUED BY **Cirrus Research**

DATE OF ISSUE **13 February 2025** CERTIFICATE NUMBER **232798**

Page 1 of 2

Approved signatory
R.Thomas
Electronically signed:

Cirrus Research
Acoustic House
Bridlington Road
Hunmanby
North Yorkshire
YO14 0PH
United Kingdom

doseBadge Reader : IEC 60942:2003

Instrument information

Manufacturer: Cirrus Research plc **Notes:**
Model: RC:110A
Serial number: 89107
Class: 2

Test summary

Date of calibration: 12 February 2025

The doseBadge reader detailed above has been calibrated to the published data as described in the operating manual and in the half-inch configuration. The procedures and techniques used are as described in IEC60942_2003 Annex B – Periodic Tests and three determinations of the sound pressure level, frequency and total distortion were made.

The sound pressure level was measured using a WS2F concenser microphone type MK:224 manufactured by Cirrus Research plc.

The results have been corrected to the reference pressure of 101.33 kPa using the manufacturer's data.

The doseBadge Reader has been shown to conform to the Class 2 requirements for periodic testing, described in Annex B of IEC 60942:2003 for the sound pressure level(s) and frecuency(ies) stated, for the environmental conditions under which the tests were performed.

However, as public evidence was not available, from a testing organisation responsible for pattern approval, to demonstrate that the model of doseBadge Reader conformed to the requirements for pattern evaluation described in Annex A of IEC 60942:2003, no general statement or conclusion can be made about conformance of the doseBadge Reader to the requirements of IEC 60942:2003.

Notes:

REVIEW BY .....
APPROVED BY .....
NEXT CAL DATE..... 11/ 02/ 2026

This certificate provides traceability of measurement to the SI system of units and/or to units of measurement realised at the National Physical Laboratory or other recognised national metrology institutes. This certificate may not be reproduced other than in full, except with the prior written approval of the issuing laboratory. The results within this certificate relate only to the items calibrated. The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor k=2, providing a coverage probability of approximately 95%.

CERTIFICATE OF CALIBRATION

Certificate Number: **232798**

Page 2 of 2

Environmental conditions

The following conditions were recorded at the time of the test:
Before Pressure: 101.41 kPa Temperature: 24.9 °C Humidity: 32.4 %
After Pressure: 101.42 kPa Temperature: 25.0 °C Humidity: 32.7 %

Test equipment

Equipment	Manufacturer	Model	Serial number
Distortion Meter	Keithley	2015	1063074
Environmental Monitor	Comet	T7510	21962628

Acoustic Results

	Expected	Sample 1	Sample 2	Sample 3	Average	Deviation	Tolerance	Uncertainty
Level (dB)	114.00	114.00	114.01	114.00	**114.00**	0.00	±0.75	0.11 dB
Distortion (%)	< 4.00	0.98	0.70	0.72	**0.80**	0.80	+4.00	0.13 %
Frequency (Hz)	1000.0	1002.2	1002.2	1002.2	**1002.2**	2.2	±20.0	0.1 Hz

The measured quantities or deviations (as applicable), extended by the expanded combined uncertainty of measurement, must not exceed the corresponding tolerance.

Functionality Results

Function	Result
Keypad	Pass
Battery Power	Pass
Display	Pass
Communication	Pass
2 way IR link	Pass
Clock	Pass

End of results

JNAC
JIRANATEE ASSOCIATES CO.,LTD.

Jiranatee Associates Co.,Ltd
63/14-15, 17/35-36
Petchkasem 7,(7), Rd, Wanthapra, Bangkoiyai,
Nonthaburi 11000(Thailand)
Tel: +6628669813
Mobile: +66863899453
E-mail: nac-calibration@jiranatee.com
Web site: www.jiranatee.com

Accredited calibration laboratory
ISO/IEC 17025:2017
NAC 156-TN 17025
CALIBRATION 0367

Acoustic calibration laboratory
Calibration services department.

REVIEW BY .....
APPROVED BY .....
NEXT CAL DATE.... 03/ 09/ 2026

Calibration report Number
CDM-040-68

CALIBRATION REPORT

Page 1 of 1 Pages

MEASUREMENT ITEM	: Dose meter
MANUFACTURER	: Cirrus Research plc.
MODEL/TYPE	: CR:110AMS
SERIAL NUMBER	: 91472
ID NUMBER	: RYG_250033
CONDITION AS-RECEIVED	: Used item
CUSTOMER	: AGS laboratory group (thailand) Co., Ltd. 104 Phatthanakan 40, Phatthanakan Rd, Khwaeng Suan Luang, Khet Suan Luang, Bangkok 10250 Thailand.
RECEIVED DATE	: 02 Sep 2025
MEASUREMENT DATE	: 04 Sep 2025
ISSUE DATE	: 04 Sep 2025

Calibration procedures:
The Noise dosimeter (Unit Under Calibration) was calibrated against Standard doseBadge reader model: RC:110A which the calibration was performed respecting the requirements of ISO/IEC 17025:2017 and carried out in accordance with the requirements of IEC 60942:2003 where applicable.

Traceability:
This certificate provides a traceability of The measurement to recognized the national standards, and to realization of the International system of units (SI) through Cirrus research plc via Certificate Number: 248239

ENVIRONMENTAL CONDITIONS:
Ambient condition in the laboratory are as follow:

Temperature	: 23.0 ± 3.0	°C
Relative Humidity	: 55.0 ± 15.0	%RH
Atmospheric Pressure	: 1010± 10	hPa

PRECONDITIONING : The dose meter (Unit Under Calibration) was preconditioning 24 hours at ambient conditions prior to calibration being performed.

STANDARD USED DURING CALIBRATION:
Instrument name: doseBadge Reader Manufacturer: Cirrus Research plc. Model: RC:110A Serial number: 81051
Remark: doseBadge Reader Unit with Internal Acoustic Calibrator to IEC 60942:2003 Class 2.

CALIBRATION RESULTS:
Table 1: The results of dose meter calibration are reported in the table below.

DoseBadge Reader Level[1] (dB)	Noise DoseMeter reading[2] (dB)	Error (dB)	Status
114.0	114.0	0.0	✓

Calibrated by:
☒ Mr. Surawit Jitpahuled
☐ Miss Jittraporn Leesomphol

JNAC JIRANATEE ASSOCIATES CO.,LTD.

Approved signatory.....
Mr. Parinya Booncharoen
Calibration Department Manager

Remark:
[1] The decibel level of standard doseBadge reader that supplied to Unit Under Calibration.
[2] The measurement reading of Unit Under Calibration.

THIS CALIBRATION REPORT MAY NOT BE REPRODUCED EXCEPT IN FULL UNLESS PERMISSION FOR REPRODUCTION HAS BEEN OBTAINED IN WRITING FROM THE LABORATORY

CERTIFICATE OF CALIBRATION

ISSUED BY **Cirrus Research**

DATE OF ISSUE **13 February 2025** CERTIFICATE NUMBER **232797**

Page 1 of 2

Approved signatory
R.Thomas
Electronically signed:

Cirrus Research
Acoustic House
Bridlington Road
Hunmanby
North Yorkshire
YO14 0PH
United Kingdom

doseBadge Reader : IEC 60942:2003

Instrument information

Manufacturer: Cirrus Research plc **Notes:**
Model: RC:110A
Serial number: 73729
Class: 2

Test summary

Date of calibration: 12 February 2025

The doseBadge reader detailed above has been calibrated to the published data as described in the operating manual and in the half-inch configuration. The procedures and techniques used are as described in IEC60942_2003 Annex B – Periodic Tests and three determinations of the sound pressure level, frequency and total distortion were made.

The sound pressure level was measured using a WS2F concenser microphone type MK:224 manufactured by Cirrus Research plc.

The results have been corrected to the reference pressure of 101.33 kPa using the manufacturer's data.

The doseBadge Reader has been shown to conform to the Class 2 requirements for periodic testing, described in Annex B of IEC 60942:2003 for the sound pressure level(s) and frecuency(ies) stated, for the environmental conditions under which the tests were performed.

However, as public evidence was not available, from a testing organisation responsible for pattern approval, to demonstrate that the model of doseBadge Reader conformed to the requirements for pattern evaluation described in Annex A of IEC 60942:2003, no general statement or conclusion can be made about conformance of the doseBadge Reader to the requirements of IEC 60942:2003.

Notes:

REVIEW BY .....
APPROVED BY .....
NEXT CAL DATE..... 11/ 02/ 2026

This certificate provides traceability of measurement to the SI system of units and/or to units of measurement realised at the National Physical Laboratory or other recognised national metrology institutes. This certificate may not be reproduced other than in full, except with the prior written approval of the issuing laboratory. The results within this certificate relate only to the items calibrated. The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor k=2, providing a coverage probability of approximately 95%.

CERTIFICATE OF CALIBRATION

Certificate Number: **232797**

Page 2 of 2

Environmental conditions

The following conditions were recorded at the time of the test:
Before Pressure: 101.42 kPa Temperature: 25.1 °C Humidity: 33.1 %
After Pressure: 101.42 kPa Temperature: 25.2 °C Humidity: 35.9 %

Test equipment

Equipment	Manufacturer	Model	Serial number
Distortion Meter	Keithley	2015	1063074
Environmental Monitor	Comet	T7510	21962628

Initial Acoustic Results

	Expected	Sample 1	Sample 2	Sample 3	Average	Deviation	Tolerance	Uncertainty
Level (dB)	114.00	112.51	112.45	112.61	**112.52**	-1.48	±0.75	0.11 dB
Distortion (%)	< 4.00	1.46	1.70	2.01	**1.72**	1.72	+4.00	0.13 %
Frequency (Hz)	1000.0	998.2	998.2	998.2	**998.2**	-1.8	±20.0	0.1 Hz

The measured quantities or deviations (as applicable), extended by the expanded combined uncertainty of measurement, must not exceed the corresponding tolerance.

Adjusted Acoustic Results

	Expected	Sample 1	Sample 2	Sample 3	Average	Deviation	Tolerance	Uncertainty
Level (dB)	114.00	114.00	113.99	114.01	**114.00**	0.00	±0.75	0.11 dB
Distortion (%)	< 4.00	0.97	0.96	0.95	**0.96**	0.96	+4.00	0.13 %
Frequency (Hz)	1000.0	998.1	998.1	998.1	**998.1**	-1.9	±20.0	0.1 Hz

Functionality Results

Function	Result
Keypad	Pass
Battery Power	Pass
Display	Pass
Communication	Pass
2 way IR link	Pass
Clock	Pass

End of results

JIRANATEE ASSOCIATES CO.,LTD.

Jiranatee Associates Co.,Ltd
63/14-15, 67/35-36
Petchkasem 7,7/1, Rd. Wattharpa, Bangkokyai,
Bangkok 10600(Thailand)
Tel: +66(0)3393453
Mobile: +66(0)3393453
E-mail: jnac-calibration@jiranatee.com
Web site: www.jiranatee.com

Accredited calibration laboratory
ISO/IEC 17025:2017
NSC-TISI-TIS 17025
CALIBRATION 0367

Acoustic calibration laboratory
Calibration services department.

REVIEW BY .....
APPROVED BY.....
NEXT CAL DATE.03/ 09/ 2026

Calibration report Number
COM-045-68

CALIBRATION REPORT

Page 1 of 1 Pages

MEASUREMENT ITEM	: Dose meter	
MANUFACTURER	: Lutus research plc	
MODEL/TYPE	: CR.110AIS	
SERIAL NUMBER	: YF477	
ID NUMBER	: RYG_FS0338	
CONDITION AS-RECEIVED	: Used item	
CUSTOMER	: ALS laboratory group (thailand) Co., Ltd. 104 Phatthanakan 40, Phatthanakan Rd, Khwaeng Suan luang, Khet Suan Luang, Bangkok 10250 Thailand.	
RECEIVED DATE	: 02 Sep 2025	
MEASUREMENT DATE	: 04 Sep 2025	
ISSUE DATE	: 04 Sep 2025	

Calibration procedure:
The dose meter (Unit Under Calibration) was calibrated against Standard doseBadge reader model: RC-110A which the calibration was performed respecting the requirements of ISO/IEC 17025:2017 and carried out in accordance with the requirements of IEC 60942:2003 where applicable.

Traceability:
This certificate provides a traceability of The measurement to recognized the national standard, and to realization of the international system of units (SI) through Cirrus research plc via Certificate Number: 248239

ENVIRONMENTAL CONDITIONS:
Ambient condition in the laboratory are as follow:

Temperature	: 23.0 ± 3.0	°C
Relative Humidity	: 55.0 ± 15.0	%RH
Atmospheric Pressure	: 1010± 10	hPa

PRECONDITIONING : The dose meter (Unit Under Calibration) was preconditioning 24 hours at ambient conditions prior to calibration being performed.

STANDARD USED DURING CALIBRATION:

Instrument name:	doseBadge Reader	Manufacturer:	Cirrus Research plc	Model:	RC110A	Serial number:	B1051

Remark: doseBadge Reader Unit with Internal Acoustic Calibrator to IEC 61042: 2003 Class 2.

CALIBRATION RESULTS:
Table 1: The results of dose meter calibration are reported in the table below.

DoseBadge Reader Level[1] (dB)	Noise Dosimeter reading[2] (dB)	Error (dB)	Status
114.0	114.0	0.0	✓

Calibrated by:
☐ Mr. Sorawit Thachalad
☐ Miss Jittraporn Lertsomphol

Approved signatory: .....
Mr. Parinya Booncharoen
Calibration Department Manager

Remark:
[1] The decibel level of standard doseBadge reader that supplied to Unit Under Calibration.
[2] The measurement reading of Unit Under Calibration.

THIS CALIBRATION REPORT MAY NOT BE REPRODUCED EXCEPT IN FULL UNLESS PERMISSION FOR REPRODUCTION HAS BEEN OBTAINED IN WRITING FROM THE LABORATORY

JIRANATEE ASSOCIATES CO.,LTD.

Jiranatee Associates Co.,Ltd
63/14-15, 67/35-36
Petchkasem 7,7/1, Rd. Wattharpa, Bangkokyai,
Bangkok 10600(Thailand)
Tel: +66(0)3393453
Mobile: +66(0)3393453
E-mail: jnac-calibration@jiranatee.com
Web site: www.jiranatee.com

Accredited calibration laboratory
ISO/IEC 17025:2017
NSC-TISI-TIS 17025
CALIBRATION 0367

Temperature measurement laboratory
Calibration services department.

ilac-MRA APLAC MRA
NSC – TISI – TIS 17025
CALIBRATION 0367

CERTIFICATE OF CALIBRATION

Certificate No. : CDT-144-67

Page 1 of 2 Pages

MEASUREMENT ITEM	: Heat Stress Monitor
MANUFACTURER	: Delta OHM
MODEL/TYPE	: HD32.2
SERIAL NUMBER	: 22016390
ID NUMBER	: RYG_FS0580
CONDITION AS-RECEIVED	: Used item
CUSTOMER	: ALS laboratory group (thailand) Co., Ltd. 104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Suan Luang, Khet Suan Luang, Bangkok 10250 Thailand.
RECEIVED DATE	: 19 Jul 2024
MEASUREMENT DATE	: 07 Aug 2024
ISSUE DATE	: 07 Aug 2024

Calibration procedure:
The temperature calibration was done by In-House calibration method as WHCL-001 according to comparison method with standard digital temperature indicator and standard temperature probe. The temperature scale use was based on ITS-90.

Traceability:
The measurement results are traceable to the International system of units (SI) through National Institute of Metrology Thailand (NIMT) Certificate number: TT-0047-24, Certificate number: EA-0101-23

Reference Used During Calibration:
1. Standard Temperature Probe
Model: STS-100 A500, Serial No.: 667682-09, Due date: 26 Mar 2025
2. Digital Temperature Indicator
Model: DTI-1000-A MK II, Serial No.: 671407-00591 Due date: 14 Sep 2024

Uncertainty of Measurement:
The reported uncertainty of measurement is based on the standard uncertainty multiplied by a coverage factor k=2, Which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty has been determined in accordance with the GUM "Evaluation of measurement data - Guide to the expression of uncertainty in measurement"

ENVIRONMENTAL CONDITIONS:
Ambient condition in the laboratory are as follow:

Temperature	: 23.0 ± 3.0	°C
Relative Humidity	: 55.0 ± 15.0	%RH

NOTED: The certificate is valid only to the item calibrated on date and place of calibration.

TABULATION OF RESULTS:
The table on next page give the measured values.

REVIEW BY .....
APPROVED BY .....
NEXT CAL. DATE 9/6/25

Calibrated by:
☐ Mr. Sorawit Thachalad
☑ Miss Jittraporn Lertsomphol
☐ Miss Ruangrumpai Phoommit

Approved signatory: .....
Mr. Parinya Booncharoen
Calibration Department Manager

THIS CERTIFICATE MAY NOT BE REPRODUCED EXCEPT IN FULL UNLESS PERMISSION FOR REPRODUCTION HAS BEEN OBTAINED IN WRITING FROM THE LABORATORY

JIRANATEE ASSOCIATES CO.,LTD.

Continuation of Certificate of Calibration Number CDT-144-67

Page 2 of 2 Pages

Result of Calibration: ☑ Without Adjustment ☐ With Adjustment

Calibration Range: 20 °C to 40 °C

Function:

Table 1: This equipment was connected with wet bulb probe Model: HP3201.2 S/N: 22025580.
Dimension: Diameter 3.3 mm. Length 170 mm.

Immersion Depth (mm)	Standard Reading (°C)	UUC Reading (°C)	Error (°C)	Uncertainty (°C)
80	20.059	20.0	-0.1	0.099
80	25.054	25.0	-0.1	0.099
80	30.045	30.0	0.0	0.099
80	35.036	34.9	-0.1	0.099
80	40.027	39.9	-0.1	0.099

Table 2: This equipment was connected with Globe thermometer probe Model: TP3276.2 S/N: 22023942.
Dimension: Diameter 3.3 mm. Length 205 mm.

Immersion Depth (mm)	Standard Reading (°C)	UUC Reading (°C)	Error (°C)	Uncertainty (°C)
110	20.059	20.1	0.0	0.099
110	25.054	25.1	0.0	0.099
110	30.045	30.1	0.1	0.099
110	35.037	35.0	0.0	0.099
110	40.027	40.0	0.0	0.099

Table 3: This equipment was connected with temperature probe Model: TP3207.2 S/N: 22025040.
Dimension: Diameter 14 mm. Length 150 mm.

Immersion Depth (mm)	Standard Reading (°C)	UUC Reading (°C)	Error (°C)	Uncertainty (°C)
75	20.059	20.1	0.0	0.099
75	25.054	25.0	-0.1	0.099
75	30.045	29.9	-0.1	0.099
75	35.037	34.9	-0.1	0.099
75	40.027	39.8	-0.2	0.099

UUC*: Unit Under Calibration

End of Certificate of Calibration

THIS CERTIFICATE MAY NOT BE REPRODUCED EXCEPT IN FULL UNLESS PERMISSION FOR REPRODUCTION HAS BEEN OBTAINED IN WRITING FROM THE LABORATORY

JIRANATEE ASSOCIATES CO.,LTD.

Jiranatee Associates Co.,Ltd
63/14-15, 67/35-36
Petchkasem 7,7/1, Rd. Wattharpa, Bangkokyai,
Bangkok 10600(Thailand)
Tel: +66(0)3393453
Mobile: +66(0)3393453
E-mail: jnac-calibration@jiranatee.com
Web site: www.jiranatee.com

Accredited calibration laboratory
ISO/IEC 17025:2017
NSC-TISI-TIS 17025
CALIBRATION 0367

Temperature measurement laboratory
Calibration services department.

ilac-MRA APLAC MRA
NSC – TISI – TIS 17025
CALIBRATION 0367

CERTIFICATE OF CALIBRATION

Certificate No. : CDT-142-67

Page 1 of 2 Pages

MEASUREMENT ITEM	: Heat Stress Monitor
MANUFACTURER	: Delta OHM
MODEL/TYPE	: HD32.2
SERIAL NUMBER	: 22016388
ID NUMBER	: RYG_FS0578
CONDITION AS-RECEIVED	: Used item
CUSTOMER	: ALS laboratory group (thailand) Co., Ltd. 104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Suan Luang, Khet Suan Luang, Bangkok 10250 Thailand.
RECEIVED DATE	: 19 Jul 2024
MEASUREMENT DATE	: 06 Aug 2024
ISSUE DATE	: 07 Aug 2024

Calibration procedure:
The temperature calibration was done by In-House calibration method as WHCL-001 according to comparison method with standard digital temperature indicator and standard temperature probe. The temperature scale use was based on ITS-90.

Traceability:
The measurement results are traceable to the International system of units (SI) through National Institute of Metrology Thailand (NIMT) Certificate number: TT-0047-24, Certificate number: EA-0101-23

Reference Used During Calibration:
1. Standard Temperature Probe
Model: STS-100 A500, Serial No.: 667682-09, Due date: 26 Mar 2025
2. Digital Temperature Indicator
Model: DTI-1000-A MK II, Serial No.: 671407-00591 Due date: 14 Sep 2024

Uncertainty of Measurement:
The reported uncertainty of measurement is based on the standard uncertainty multiplied by a coverage factor k=2, Which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty has been determined in accordance with the GUM "Evaluation of measurement data - Guide to the expression of uncertainty in measurement"

ENVIRONMENTAL CONDITIONS:
Ambient condition in the laboratory are as follow:

Temperature	: 23.0 ± 3.0	°C
Relative Humidity	: 55.0 ± 15.0	%RH

NOTED: The certificate is valid only to the item calibrated on date and place of calibration.

TABULATION OF RESULTS:
The table on next page give the measured values.

REVIEW BY .....
APPROVED BY .....
NEXT CAL. DATE 6/1/25

Calibrated by:
☐ Mr. Sorawit Thachalad
☑ Miss Jittraporn Lertsomphol
☐ Miss Ruangrumpai Phoommit

Approved signatory: .....
Mr. Parinya Booncharoen
Calibration Department Manager

THIS CERTIFICATE MAY NOT BE REPRODUCED EXCEPT IN FULL UNLESS PERMISSION FOR REPRODUCTION HAS BEEN OBTAINED IN WRITING FROM THE LABORATORY

JIRANATEE ASSOCIATES CO.,LTD.

Continuation of Certificate of Calibration Number CDT-142-67

Page 2 of 2 Pages

Result of Calibration: ☑ Without Adjustment ☐ With Adjustment

Calibration Range: 20 °C to 40 °C

Function:

Table 1: This equipment was connected with wet bulb probe Model: HP3201.2 S/N: 22015694.
Dimension: Diameter 3.3 mm. Length 170 mm.

Immersion Depth (mm)	Standard Reading (°C)	UUC Reading (°C)	Error (°C)	Uncertainty (°C)
80	20.059	19.9	-0.2	0.099
80	25.054	24.9	-0.2	0.099
80	30.047	29.9	-0.1	0.099
80	35.036	34.9	-0.1	0.099
80	40.029	39.8	-0.2	0.099

Table 2: This equipment was connected with Globe thermometer probe Model: TP3276.2 S/N: 22023956.
Dimension: Diameter 3.3 mm. Length 205 mm.

Immersion Depth (mm)	Standard Reading (°C)	UUC Reading (°C)	Error (°C)	Uncertainty (°C)
110	20.060	20.1	0.0	0.099
110	25.054	25.1	0.0	0.099
110	30.047	30.1	0.1	0.099
110	35.036	35.1	0.1	0.099
110	40.029	40.1	0.1	0.099

Table 3: This equipment was connected with temperature probe Model: TP3207.2 S/N: 22025031.
Dimension: Diameter 14 mm. Length 150 mm.

Immersion Depth (mm)	Standard Reading (°C)	UUC Reading (°C)	Error (°C)	Uncertainty (°C)
75	20.059	20.2	0.1	0.099
75	25.053	25.1	0.0	0.099
75	30.047	30.0	-0.1	0.16
75	35.036	34.9	-0.1	0.099
75	40.029	39.8	-0.2	0.099

UUC*: Unit Under Calibration
Remark: The reported uncertainty of measurement is 0.16, based on standard uncertainty multiplied by a coverage factor k=2.21 providing a level of confidence of approximately 95%.

End of Certificate of Calibration

THIS CERTIFICATE MAY NOT BE REPRODUCED EXCEPT IN FULL UNLESS PERMISSION FOR REPRODUCTION HAS BEEN OBTAINED IN WRITING FROM THE LABORATORY

JIRANATEE ASSOCIATES CO.,LTD.

Jiranatee Associates Co.,Ltd
63/14-15, 67/35-36
Petchkasem 7,7/1, Rd. Wattharpa, Bangkokyai,
Bangkok 10600(Thailand)
Tel: +66(0)3393453
Mobile: +66(0)3393453
E-mail: jnac-calibration@jiranatee.com
Web site: www.jiranatee.com

Accredited calibration laboratory
ISO/IEC 17025:2017
NSC-TISI-TIS 17025
CALIBRATION 0367

Temperature measurement laboratory
Calibration services department.

ilac-MRA APLAC MRA
NSC – TISI – TIS 17025
CALIBRATION 0367

CERTIFICATE OF CALIBRATION

Certificate No. : CDT-069-68

Page 1 of 2 Pages

MEASUREMENT ITEM	: Heat Stress Monitor
MANUFACTURER	: Delta OHM
MODEL/TYPE	: HD32.2
SERIAL NUMBER	: 20032249
ID NUMBER	: RYG_FS0524
CONDITION AS-RECEIVED	: Used item
CUSTOMER	: ALS laboratory group (thailand) Co., Ltd. 104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Suan Luang, Khet Suan Luang, Bangkok 10250 Thailand.
RECEIVED DATE	: 03 Mar 2025
MEASUREMENT DATE	: 18 Mar 2025
ISSUE DATE	: 20 Mar 2025

Calibration procedure:
The temperature calibration was done by In-House calibration method as WHCL-001 according to comparison method with standard digital temperature indicator and standard temperature probe. The temperature scale use was based on ITS-90.

Traceability:
The measurement results are traceable to the International system of units (SI) through National Institute of Metrology Thailand (NIMT) Certificate number: TT-0047-24, Certificate number: EA-0113-24

Reference Used During Calibration:
1. Standard Temperature Probe
Model: STS-100 A500, Serial No.: 667682-09, Due date: 26 Mar 2025
2. Digital Temperature Indicator
Model: DTI-1000-A MK II, Serial No.: 671407-00591 Due date: 21 Oct 2025

Uncertainty of Measurement:
The reported uncertainty of measurement is based on the standard uncertainty multiplied by a coverage factor k=2, Which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty has been determined in accordance with the GUM "Evaluation of measurement data - Guide to the expression of uncertainty in measurement"

ENVIRONMENTAL CONDITIONS:
Ambient condition in the laboratory are as follow:

Temperature	: 23.0 ± 3.0	°C
Relative Humidity	: 55.0 ± 15.0	%RH

NOTED: The certificate is valid only to the item calibrated on date and place of calibration.

TABULATION OF RESULTS:
The table on next page give the measured values.

REVIEW BY .....
APPROVED BY .....
17/ 03/ 2026
NEXT CAL DATE.....

Calibrated by:
☐ Mr. Sorawit Thachalad
☑ Miss Jittraporn Lertsomphol
☐ Miss Ruangrumpai Phoommit

Approved signatory: .....
Mr. Parinya Booncharoen
Calibration Department Manager

THIS CERTIFICATE OF CALIBRATION MAY NOT BE REPRODUCED EXCEPT IN FULL UNLESS PERMISSION FOR REPRODUCTION HAS BEEN OBTAINED IN WRITING FROM THE LABORATORY

JIRANATEE ASSOCIATES CO.,LTD.

Continuation of Certificate of Calibration Number CDT-069-68

Page 2 of 2 Pages

Result of Calibration: ☑ Without Adjustment ☐ With Adjustment

Calibration Range: 20 °C to 40 °C

Function:

Table 1: This equipment was connected with wet bulb probe Model: HP3201.2, S/N: 21001215.
Dimension: Diameter 3.3 mm. Length 170 mm.

Immersion Depth (mm)	Standard Reading (°C)	UUC Reading (°C)	Error (°C)	Uncertainty (°C)
80	20.056	20.2	0.1	0.099
80	25.050	25.2	0.2	0.099
80	30.034	30.2	0.2	0.099
80	35.018	35.2	0.2	0.099
80	39.996	40.1	0.1	0.099

Table 2: This equipment was connected with Globe thermometer probe Model: TP3276.2, S/N: 21001244.
Dimension: Diameter 3.3 mm. Length 205 mm.

Immersion Depth (mm)	Standard Reading (°C)	UUC Reading (°C)	Error (°C)	Uncertainty (°C)
110	20.056	20.0	-0.1	0.099
110	25.050	25.0	0.0	0.099
110	30.034	30.0	0.0	0.099
110	35.018	35.0	0.0	0.099
110	39.996	40.0	0.0	0.099

Table 3: This equipment was connected with temperature probe Model: TP3207.2, S/N: 21001790.
Dimension: Diameter 14 mm. Length 150 mm.

Immersion Depth (mm)	Standard Reading (°C)	UUC Reading (°C)	Error (°C)	Uncertainty (°C)
75	20.056	20.1	0.0	0.099
75	25.050	25.0	0.0	0.099
75	30.034	29.9	-0.1	0.099
75	35.018	34.9	-0.1	0.099
75	39.996	39.8	-0.2	0.099

UUC*: Unit Under Calibration

End of Certificate of Calibration

THIS CERTIFICATE OF CALIBRATION MAY NOT BE REPRODUCED EXCEPT IN FULL UNLESS PERMISSION FOR REPRODUCTION HAS BEEN OBTAINED IN WRITING FROM THE LABORATORY

TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000-29 FAX 0-2719-9484

ilac-MRA APLAC MRA
NSC-TISI-TIS17025
CALIBRATION 0008

Certificate of Calibration

Cert.No.: 25CH847
Page.: 1 of 3

Equipment :	pH Meter
Manufacturer :	Mettler Toledo
Model :	SevenCompact S220
Serial No. :	C104059460
ID No. :	RYG_EN0183
Condition As-Received:	Used Item
Received Date :	17 July 2025
Calibration Date :	18 July 2025
Reference :	2507-0561DSC-3
Submitted by :	ALS Laboratory Group (Thailand) Co.,Ltd. Rayong Branch 616/10 Moo 5, T.Maenam Khu, A.Pluakdaeng, Rayong 21140, Thailand
Ambient Temperature :	(25 ± 2.5) °C
Relative Humidity :	(50 ± 15) %
Calibration Procedure :	In - house method : - CP-CH5 by direct measurement with DC voltage standard and direct measurement with certified reference material (CRM) - CP-CH8 by comparison with temperature standard

REVIEW BY .....Phatchana S.
APPROVED BY.....
NEXT CAL DATE.....18/01/27

Calibrated by : Walalak Sirithean

Approved by : Saithip
Approved Signatory

( ) Chakrit Waewwanjua
( ) Ponpan Paipim
(✓) Saithip Meangmai

Issue Date : 21 July 2025

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

Cert.No.: 25CH847
Page.: 2 of 3

Condition of this calibration result

1. Reference Standard Instrument

Instrument	Serial No.	ID No.	Cert. No.	Due Date
1) Document Process Calibrator	54030049	130RC116	24E2759	25 Aug 2025
2) Ref. Standard Thermometer	324C076	60RC033	25I394	01 Apr 2026

- This measurement result is traceable to SI throught Technology Promotion Association (Thailand - Japan)

2. Certified Reference Materials : The measurement results are traceable to SI through CPA chem Ltd., ANSI-ASQ National Accreditation Board, Accredited No. AR-1835

Buffer Solution	Manufacturer	Lot No.	Exp. date
pH 4.007	CPA chem	1066665	18 Jan 2027
pH 6.965	CPA chem	1066667	18 Jan 2026
pH 10.010	CPA chem	1114385	08 June 2026

3. This certificate is valid only to the item calibrated on date and place of calibration.

Calibration Results

Function : mV Measurement

Performing standard curve by Document Process Calibrator at pH (4,7,10)

Unit Under Calibration	Nominal Value	Standard Voltage Input	Actual Reading		Uncertainty of Measurement	Coverage factor
	pH	mV	mV	pH	(±mV)	k
pH Meter	4.000	177.48	177.3	4.000	0.058	2.00
S/N.: C104059460	7.000	0.00	-0.2	7.000	0.058	2.00
	10.000	-177.48	-177.6	10.000	0.058	2.00

Cert.No.: 25CH847
Page.: 3 of 3

Calibration Results

Function : pH Measurement

Performing three buffers standard curve by using buffer nominal pH (4,7,10)

Unit Under Calibration	Standard pH Buffer Solution	Actual pH Reading	Actual mV Reading (mV)	Uncertainty of pH Measurement (±)	Coverage factor *k*
pH Electrode	4.007	4.008	184.6	0.0044	2.00
S/N.: 5240606	6.965	6.966	10.2	0.0084	2.00
	10.010	10.009	-164.9	0.0065	2.00

Function : Temperature Measurement

(*) Without adjustment

This equipment was connected with Temperature Probe;

- Model : InLabExpert Pro-ISM
- Serial No. : 5240606

Dimension of probe

- Length : 120 mm.
- Diameter : 12 mm.
- Immersion Depth : 100 mm.

Calibration Point (°C)	Standard Temperature (°C)	UUC* Reading (°C)	Error (°C)	Uncertainty of measurement (± °C)	Coverage factor *k*
25.0	25.001	25.0	-0.001	0.13	2.00

Remark - UUC* = Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000-24 FAX. 0-2719-9484

NSC-TISI-TIS17025 CALIBRATION 0008

Certificate of Calibration

Certificate No. : 25E2372
Page : 1 of 2

Equipment : pH Meter
Manufacturer: Mettler Toledo
Model : SevenCompact S220
Serial No.: C104059460
ID No.: RYG_EN0183
Condition As-Received: Used Item
Received Date: 17 July 2025
Calibration Date: 22 July 2025
Reference: 2507-0561DSC
Ambient Temperature: (23 ± 2) °C
Relative Humidity: (50 ± 10) %

This certificate may not be reproduced other than in full, except with the prior written approval of the head of Corporate Services 3: Equipment Calibration and Testing Services.

Submitted by: ALS Laboratory Group (Thailand) Co.,Ltd. Rayong Branch
616/10 Moo 5, T.Maenam Khu, A.Pluakdaeng, Rayong 21140, Thailand

Procedure used: Calibration were conducted using calibration procedure No. CP-E17 according to EURAMET cg-15.

Condition of this result of calibration

1.Reference standards instruments :

Instrument	Model	Serial No.	Certificate No.	Due Date
1) Multi-Product Calibrator	5500A	6315011	25E1627	19 May 2026

2.This result of calibration was made on requested at the point specified by customer.
3.The certificate is valid only to the item calibrated on date and place of calibration.
4.This measurement result is traceable to the International System of Unit maintained through:-
-Technology Promotion Association (Thailand-Japan), NSC-ONSC Accredited No. Calibration 0008

Calibrated by : Napachanok Prasomsoosiri
Issue Date : 23 July 2025

Approved Signatory :
[ ] Phalinee Prabpaiphat
[ ] Nuntawat Khamchai
[√] Pongsagorn Boonyaporn

Cert. No.: 25E2372
Page.: 2 of 2

Result of calibration :- (*) Without adjustment ( ) After adjustment

Function: DC voltage measurement **Range:** 2000 mV

Standard Value (mV)	UUC* Reading (mV)	Error (mV)	Uncertainty (± μV)
-200.0000	-200.0	0.0	68
-150.0000	-150.0	0.0	65
-100.0000	-100.0	0.0	63
-50.0000	-50.0	0.0	61
0.0000	0.0	0.0	58
50.0000	49.9	-0.1	61
100.0000	99.9	-0.1	63
150.0000	149.9	-0.1	65
200.0000	199.9	-0.1	68

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k* = 2, providing a level of confidence of approximately 95 %.

UUC* = Unit Under Calibration.

-o0o-

TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL.0-2717-3000-29 FAX.3-2719-9484

NSC-TISI-TIS17025 CALIBRATION 0008

Certificate of Calibration

Cert. No.: 25LM10
Page.: 1 of 2

Equipment : DO Meter with Sensor
Manufacturer : YSI
Model : 5000-115V
Serial No. : 15E102796
ID No. : RYG_EN0032

REVIEW BY ..... Photchanna S.
APPROVED BY ..... D Sumitra
NEXT CAL DATE..... 20/07/26

Submitted by : ALS Laboratory Group (Thailand) Co.,Ltd. (Rayong Branch) 616/10 Moo 5 T. Maenam Khu, A. Pluakdaeng, Rayong 21140 Thailand

Location : TPA On Site Calibration Laboratory

Received Order : 17 January 2025
Calibrated Date : 20 January 2025
Ambient Temperature : (26 ± 10) °C
Relative Humidity : (50 ± 30) %
AC Line Voltage : (220 ± 22) V

Calibrated by : Warakorn Lemgagtrakul

Approved by : Approved Signatory

( ) Chakrit Waewwanjua
(√) Suwit Imjai
( ) Kunchit Promprat

Issue Date : 23 January 2025

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

Equipment : DO Meter with Sensor
Condition As-Received : Used Item
Reference : 2501-0600DSC-2

Cert. No.: 25LM10
Page.: 2 of 2

Procedure Used :-

Calibration were conducted using in-house calibration procedure CP-OT01 according to comparison with Industrial Platinum Resistance Thermometer (IPRT) into Temperature Bath.
The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

Instrument	Serial No.	Cert. No.	Traceable	Due Date
1) Digital Thermometer	2180080	24I1222	TPA	17 Sep 2025

2. This certificate is valid only to the item calibrated on date and place of calibration.
3. This certification is traceable to the International System of Unit.
Remark : TPA : Technology Promotion Association (Thailand - Japan)

Result of Calibration :- (*) Without Adjustment
Function : Temperature measurement.
This instrument was connected with temperature sensor, S/N.: 15E100464

Calibration Point (°C)	Immersion Depth (mm)	Standard Temperature (°C)	UUC* Reading (°C)	Error (°C)	Uncertainty (± °C)	Coverage Factor *k*
20.00	60	20.002	19.81	-0.192	0.15	2.00

UUC* : Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of aproximately 95 %.

-o0o-

TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3 : EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000 FAX. 0-2719-9484

Certificate of Testing

Cert.No.: [redacted]
Page.: [redacted]

Equipment : [redacted]
Manufacturer : [redacted]
Model : [redacted]
Serial No. : [redacted]
ID No. : [redacted]
Received Date : [redacted]
Test Date : [redacted]
Reference : [redacted]
Submitted by : [redacted]
Laboratory Condition : [redacted]
Test Procedure : [redacted]
Tested by : [redacted]
Approved by : Saithip
[redacted]
Issue Date : [redacted]

Cert.No.: [redacted]
Page.: [redacted]

Condition of this result of calibration

[redacted]

Instruments	Serial No.	ID No.	Certificate No.	Due Date
[redacted]	[redacted]	[redacted]	[redacted]	[redacted]

Material	Manufacturer	Lot.No.	Assay
[redacted]	[redacted]	[redacted]	[redacted]

Result : **Dissolved Oxygen Meter Adjustment With Air 100 %**
Dissolved Oxygen Probe No.: [redacted]

Titration Method (Azide Modification Method)	DO Meter Reading	Standard Deviation
[redacted]	[redacted]	[redacted]
[redacted]	[redacted]	[redacted]

[redacted]

-o0o-

TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL.0-2717-3000-29 FAX.3-2719-9484

NSC-TISI-TIS17025 CALIBRATION 0008

Certificate of Calibration

Cert. No.: 24TM1663
Page : 1 of 3

Equipment : Low Temp. Incubator
Manufacturer : Memmert
Model : IPP750
Serial No. : V818.0084
ID No. : RYG_EN0154

REVIEW BY ..... Thanitak.
APPROVED BY ..... D Sumitra
NEXT CAL DATE..... 01/05/26

Submitted by : ALS Laboratory Group (Thailand) Co.,Ltd. Rayong Branch 616/10 Moo 5, T.Maenam Khu, A.Pluakdaeng. Rayong 21140, Thailand

Location : BOD Room

Received Order : 01 November 2024
Calibration Date : 01 November 2024
Ambient Temperature : (26 ± 10) °C
Relative Humidity : (50 ± 30) %
AC Line Voltage : (220 ± 22) V

Calibrated by : Krisda Malee

Approved by : Approved Signatory

( ) Ponpan Paipim
( ) Suwit Imjai
(√) Kunchit Promprat

Issue Date : 07 November 2024

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

Equipment : Low Temp. Incubator
Condition As-Received : Used Item
Reference : 2411-0002OC-1

Cert. No.: 24TM1663
Page : 2 of 3

Procedure Used :-

Calibration were conducted using calibration procedure CP-OT02 based on TLAS G-20 according to direct measurement method with Data Acquisition which connected with Resistance Temperature Detector (RTD).
The temperature scale used was based on ITS-90.

Condition of this result of calibration


1. Reference standard instrument:-

Instrument	Serial No.	Cert. No.	Traceable	Due Date
1) Data Acquisition	MY44073381	24LM73	TPA	18 May 2025

2. This certificate is valid only to the item calibrated on date and place of calibration.
3. This certification is traceable to the International System of Unit.
Remark : TPA : Technology Promotion Association (Thailand - Japan)

Result of Calibration :- (*) Without Adjustment
Function of UUC* : Temperature Source
Fresh air setting : Close

Environment during calibration	Beginning	Finished
Temp. (°C)	24	25
REL.Humid. (%)	55	53
AC Supply (Volt)	220	221



Position :	Ref. Std. ID No.:
1	1RTD-2/1
2	1RTD-2/2
3	22-01RTD-03
4	1RTD-2/4
5	1RTD-2/5
6	1RTD-2/6
7	23-01RTD-07
8	1RTD-2/8
9 (ref.)	23-01RTD-09

Probe Installation Details :
a = 10 cm
b = 10 cm
c = 10 cm

Dimension of Chamber :
D = 0.60 m
W = 1.0 m
H = 1.2 m
Capacity = 0.72 m³

Equipment : Low Temp. Incubator
Condition As-Received : Used Item
Reference : 2411-0002OC-1
Result of Calibration :- (*) Without Adjustment
Function of UUC* : Temperature Source
Fresh air setting : Close

Cert. No.: 24TM1663

Calibration Point (°C)	UUC* Setting (°C)	UUC* Reading (°C)	Temperature stability (± °C)	Temperature uniformity (°C)	Overall Variation (°C)	Coverage Factor *k*
20.0	20.0	20.0	0.026	0.26	0.53	2

Calibration Point	Measured Temperature (°C) Position									Uncertainty
(°C)	1	2	3	4	5	6	7	8	9 (ref.)	(±°C)
20.0	20.071	19.915	20.273	20.179	19.977	19.782	20.056	20.026	20.033	0.30

Average* : The average of 30 values in each position.
Temperature stability : One-half of the greatest maximum difference of measured temperature at any one sensor.
Temperature uniformity : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.
Overall Variation : The Difference of the maximum and minimum measured temperatures throughout observation.
UUC* : Unit Under Calibration
Note : The reported uncertainty of measurement was included stability and excluded uniformity .

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-c0o-

SARTORIUS

Accredited by
NSC-TISI-TIS 17025
Calibration 0426

Calibration certificate

Calibration Certificate No. 25BKL0002

Object	Electronic non-automatic weighing instrument	This calibration certificate documents the traceability to national standards.
Manufacturer	Sartorius	Uncertainties of measurements are taken into account when only statements of compliance are made.
Type	MCE224S-2S00-U	This certificate was prepared by Sartorius Corporation in accordance to the current ISO/IEC 17025:2017 standard and Sartorius Work Instruction (Method) SOP WI 08.
Serial | QM Ident. no.	38101399 | RYG_EN0163	This certificate relate and apply this equipment only.
Customer	ALS Laboratory Group (Thailand) Co.,Ltd. (Rayong Branch) 616/10 Moo 5 T.Maenam Khu, A.Pluak Daeng, Rayong 21140, Thailand.	REVIEW BY Thanitak. APPROVED BY D.Sumrao NEXT CAL DATE 20/02/26
Order no.	2230	
Number of pages	4	
Date of calibration	20 Feb 2025	

This calibration certificate may not be reproduced other than in full except with the permission of NSC-TISI-TIS-17025 and the issuing laboratory. Calibration certificates without signature are not valid.

The user is obliged to have the object recalibrated at appropriate intervals.

Date	Approval of the Calibration Certificate	Person in charge
06 Mar 2025	Mr. Chonchai Inthana	Kachen Lalee

Calibration object

Single range instrument

Model	MCE224S-2S00-U
Serial Number	38101399
QM Ident. no | Inventory no	RYG_EN0163 | ---
Maximum capacity (Max. load)	220.0000 g
Measured range	220.0000 g
Scale interval	0.0001 g

Place of calibration

Address	According to page 1
Department | Cost center	Laboratory Department. | ---
Building | Floor	--- | 1st Floor.
Room	Balance Room.
Maximum temperature variation at place of calibration	5 K

Calibration procedure

EURAMET cg-18, V4.0 - Guidelines on the Calibration of Non-Automatic Weighing Instruments

Test equipment

Test equipment type	Test equipment ID	Valid until
Thermometer	MHB-382SD s/nB011342 Traceable to SI unit through DKSH	21 Aug 2025
Test weight set OIML R111 E2	Certificate No.M23081975 ,E2(Traceable to SI unit through TCS)	23 Aug 2025

Adjustment Status

The measuring device was internally adjusted before the calibration.

Environmental and measuring conditions

Date of calibration	20 Feb 2025
Temperature at place of calibration | Temp. diff. $T_{weights}$ - T_{device}	24.4 °C | 0.6 K
Measuring conditions	The installation site is suitable. The device was levelled. Balance was loaded up to Max before test.
Comments	Humidity 59.0 %RH.

Measurement results | Measurement uncertainties

Repeatability

Test load (nominal): 10 g | 200 g		
	10 g	200 g
1	10.0000 g	200.0000 g
2	10.0000 g	200.0000 g
3	10.0000 g	200.0001 g
4	9.9999 g	200.0000 g
5	9.9999 g	200.0000 g
6	10.0000 g	200.0001 g
7	10.0000 g	200.0000 g
8	10.0000 g	200.0000 g
9	9.9999 g	200.0001 g
10	10.0000 g	200.0000 g
	s = 0.00005 g	s = 0.00005 g

Eccentricity

Test load (nominal):	100 g
Center	100.0000 g
Front left	100.0000 g
Back left	100.0000 g
Back right	100.0000 g
Front right	99.9999 g
Maximum deviation from centric loading indication	
$\|\Delta E_{ecc}\|_{max}$ = 0.0001 g	

Error of indication

	Testload L	Indication I	Error E	Expansion factor k	Uncertainty U(E)	Uncertainty relative $U_{rel}(E)$
	0.0100 g	0.0100 g	0.0000 g	2.00	0.00013 g	1.3 %
	0.1000 g	0.1000 g	0.0000 g	2.00	0.00013 g	0.13 %
	0.5000 g	0.5000 g	0.0000 g	2.00	0.00013 g	0.026 %
	1.0000 g	1.0000 g	0.0000 g	2.00	0.00013 g	0.013 %
	5.0000 g	5.0000 g	0.0000 g	2.00	0.00013 g	0.0026 %
	10.0000 g	9.9999 g	-0.0001 g	2.00	0.00013 g	0.0013 %
	20.0000 g	20.0000 g	0.0000 g	2.00	0.00014 g	0.00068 %
	50.0000 g	50.0001 g	0.0001 g	2.00	0.00010 g	0.00029 %
	100.0000 g	100.0000 g	0.0000 g	2.00	0.00018 g	0.00018 %
	200.0000 g	200.0000 g	0.0000 g	2.00	0.00028 g	0.00014 %
	220.0000 g	220.0000 g	0.0000 g	2.00	0.00032 g	0.00015 %
Maximum error of indication			$\|E\|_{max}$ = 0.0001 g			

$U_{rel}(E)$ is the quotient of U(E) and test load L. The uncertainty of measurement U(E) is valid only if error E is considered. You will find reference notes on the uncertainty of measurement in use under: Appendix to the calibration certificate | Interpretation of measurement results.
Reference note: The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the documented Expansion factor, determined in accordance with the European Calibration Guideline EURAMET cg-18, V4.0. There is a 95 % probability that the value of the measurand will be in the assigned value range.

End of calibration certificate


Uncertainty of measurement in use

Device adjusted before measurement	Yes
Temperature deviation considered	1.5 K (isoCAL active)
Temperature coefficient considered	1 · 10⁻⁶/K
Uncertainty of the weighing result $U_{pi}(W)$	$U_{pi}(W) = 0.00013\ g + 1.16 \cdot 10^{-5} \cdot R$

Reference note: The current uncertainty of measurement is calculated by entering of the reading R into this formula. In relation to this, there is no need for a correction of the indication error. The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied with an Expansion factor of 2, determined in accordance with the European Calibration Guideline EURAMET cg-18, V4.0. There is a 95 % probability that the value of the measurand will be in the assigned value range.

Indication in % from max load	Net indication R	Uncertainty $U_{pi}(W)$	Uncertainty relative $U_{pi}(W)_{rel}$
1 %	2.2000 g	0.00016 g	0.0071 %
25 %	55.0000 g	0.00077 g	0.0014 %
50 %	110.0000 g	0.0014 g	0.0013 %
75 %	165.0000 g	0.0020 g	0.0012 %
100 %	220.0000 g	0.0027 g	0.0012 %

Graphic realization of the relative uncertainty of measurement | process accuracy

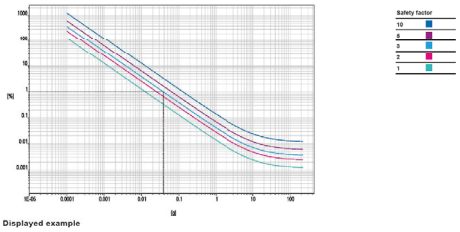

Displayed example

Process accuracy	1.00 %
Safety factor	3
Minimum sample weight	0.0381 g

SCG

Metrology Center
SCI ECO Services Company Limited
51 Moo 8, Tubkwang, Kaeng Khoi, Saraburi, Thailand 18260
Bangkok Tel : +668 9205 6851 , +669 81924 0059
Saraburi Tel : +669 8247 2360
Website : www.scieco.co.th E-Mail : calbrate@scg.co.th

NSC-TISI-TIS 17025 CALIBRATION 0244

Certificate No. T251530

Certificate of Calibration

Equipment	:	**Chamber (Oven)**
Manufacturer	:	**MEMMERT**
Model	:	**UF 110**
Serial No.	:	**B416.2420**
Customer Code	:	**RYG_EN0012**
ID No.	:	**T6444A5**
Customer	:	**ALS Laboratory Group (Thailand) Co.,Ltd. (Rayong Branch)** **616/10 Moo 5 T.Maenamkoo,** **A.Pluakdaeng, Rayong 21140**
Customer Location	:	**ENVIRONMENT LABORATORY**
Date of Receipt	:	**3 September 2025**
Calibrated By	:	**Sujjar Naknakred (Site Calibration Manager)**
Approved By	:	**Boonchai Suriyawong (Site Calibration Manager)**
Date of Issue	:	**17 SEP 2025**

REVIEW BY Thanitak.
APPROVED BY D.Sumrao
NEXT CAL. DATE 10/09/27

The uncertainties are for a confidence probability of approximately 95%.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standard laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Metrological Center.

SCG

Metrology Center
SCI ECO Services Company Limited
51 Moo 8, Tubkwang, Kaeng Khoi, Saraburi, Thailand 18260

NSC-TISI-TIS 17025 CALIBRATION 0244

Certificate No. T251530

Calibration Report

Equipment	:	**Chamber (Oven)**
Date of Calibration	:	**10 September 2025**
Environment	:	**Temperature : 35.7-36.6 °C**
		Line Voltage : 226.8-233.7 V
		Relative Humidity : 55 - 65 %RH

Condition of this results of calibration :

1. This equipment was calibrated by insert nine resistance thermometer detectors into its chamber , the other one resistance thermometer detector use for ambient temperature measurement . The calibration was done in according to WI-T20 (based on ASTM E145-94 (Reapproved 2019) and AS2853-1986).
   All data below were final values and the initial data from customer request . The temperature scale used was based on ITS - 90 .
2. Reference Standard Instrument :

Instrument	Model	Instrument No.	Certificate No.	Due Date
RTD	100 ohm	30-(CH1-10)	T242203	9 November 2025
DATA LOGGER	34970A	T47	T242203	9 November 2025

3. This certificate is traceable to :
   National Institute of Metrology (Thailand) through Metrological Center (NSC-TISI-TIS 17025 CALIBRATION 0244.
4. Condition of calibrated item : good
   Equipment Description :
   Time Constant 3 Hour 29 Minute At 104 °C
   Fresh Air Damper [X] Open [X] Min [ ] Medium [ ] Max [ ] Close [ ] Not Available
5. Adjustment :
   ( ) without adjustment (X) after adjustment

Approved By.


SCG

Metrology Center
SCI ECO Services Company Limited
51 Moo 8, Tubkwang, Kaeng Khoi, Saraburi, Thailand 18260

NSC-TISI-TIS 17025 CALIBRATION 0244

Certificate No. T251530

Calibration Report

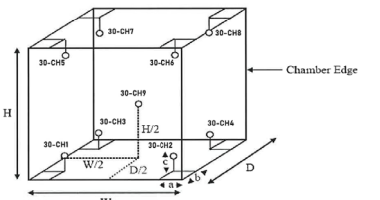

Remark : Internal Dimensions of Chamber : W (Width) = 56 cm., H (Height) = 48 cm. and D (Depth) = 40 cm.
Size of Installed Standard sensor number 30-CH1 to number 30-CH8 : a = 5 cm. ,b = 5 cm. and c = 5 cm.
Size of Installed Standard sensor number 30-CH9 : W/2 = 56 cm./2 , H/2 = 48 cm./2 and D/2 = 40cm./2

Measurement Results

Calibration Point	Average Standard Reading at each position (°C) 30-CH1	30-CH2	30-CH3	30-CH4	30-CH5	30-CH6	30-CH7	30-CH8	30-CH9
104	104.02	103.70	104.01	104.16	104.11	104.08	104.01	104.33	103.61
180	180.67	178.78	180.38	179.85	179.16	180.27	180.98	181.04	179.49

Chamber (Oven) Setting °C	Reading (°C) Min , Max	Reading (°C) Average	Temperature Distribution Average (°C)	Stability ± °C)	Uniformity (°C)	Uncertainty (± °C)	Coverage Factor *k*
104.0	103.9 , 104.1	104.0	104.00	0.08	0.61	0.42	2.00
180.0	179.9 , 180.1	180.0	180.07	0.21	1.51	0.52	2.00

* The quoted uncertainty exclude "uniformity"
The calibration result apply only the above calibrated item.
The result of test was found accurate as shown on date and place of test only.
The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor k which for a t-distribution, providing a level of confidence of approximately 95 % .

End of Certificate.

Approved By.

SARTORIUS

Accredited by
NSC-TISI-TIS 17025
Calibration 0426

Calibration certificate

Calibration Certificate No. 25BKL0003

Object	Electronic non-automatic weighing instrument	This calibration certificate documents the traceability to national standards.
Manufacturer	Sartorius	Uncertainties of measurements are taken into account when only statements of compliance are made.
Type	MSU224S-100-DU	This certificate was prepared by Sartorius Corporation in accordance to the current ISO/IEC 17025:2017 standard and Sartorius Work Instruction (Method) SOP WI 08.
Serial | QM Ident. no.	31709552 | RYG_EN0003	This certificate relate and apply this equipment only.
Customer	ALS Laboratory Group (Thailand) Co.,Ltd. (Rayong Branch) 616/10 Moo 5 T.Maenam Khu, A.Pluak Daeng, Rayong 21140, Thailand.	REVIEW BY Thanitak. APPROVED BY D.Sumrao NEXT CAL DATE 20/02/26
Order no.	2230	
Number of pages	4	
Date of calibration	20 Feb 2025	

This calibration certificate may not be reproduced other than in full except with the permission of NSC-TISI-TIS-17025 and the issuing laboratory. Calibration certificates without signature are not valid.

The user is obliged to have the object recalibrated at appropriate intervals.

Date	Approval of the Calibration Certificate	Person in charge
06 Mar 2025	Mr. Chonchai Inthana	Kachen Lalee

Calibration object

Single range instrument

Model	MSU224S-100-DU
Serial Number	31709552
OM Ident. no | Inventory no	RYG_EN0003 | ---

Maximum capacity (Max. load)	220.0000 g
Measured range	220.0000 g
Scale interval	0.0001 g

Place of calibration

Address	According to page 1
Department | Cost center	Laboratory Department. | ---
Building | Floor	--- | 1st Floor.
Room	Balance Room.
Maximum temperature variation at place of calibration	5 K

Calibration procedure

EURAMET cg-18, V4.0 - Guidelines on the Calibration of Non-Automatic Weighing Instruments

Test equipment

Test equipment type	Test equipment ID	Valid until
Thermometer	MHB-382SD s/nB011342 Traceable to SI unit through DKSH	21 Aug 2025
Test weight set OIML R111 E2	Certificate No.M23081978 ,E2(Traceable to SI unit through TCS)	23 Aug 2025

Adjustment Status

The measuring device was internally adjusted before the calibration.

Environmental and measuring conditions

Date of calibration	20 Feb 2025
Temperature at place of calibration | Temp. diff. $T_{weights}$ - T_{glass}	24.7 °C | 0.3 K
Measuring conditions	The installation site is suitable. The device was levelled. Balance was loaded up to Max before test.
Comments	Humidity 62.3 %RH.

Measurement results | Measurement uncertainties

Repeatability

Test load (nominal): 10 g | 200 g		
	10 g	200 g
1	10.0000 g	200.0000 g
2	10.0000 g	200.0001 g
3	9.9999 g	200.0000 g
4	10.0000 g	200.0000 g
5	10.0000 g	200.0001 g
6	9.9999 g	200.0000 g
7	10.0000 g	200.0000 g
8	10.0000 g	200.0000 g
9	10.0000 g	200.0000 g
10	10.0000 g	200.0001 g
	s = 0.00004 g	s = 0.00005 g

Eccentricity

Test load (nominal):	100 g
Center	100.0000 g
Front left	100.0000 g
Back left	100.0001 g
Back right	99.9999 g
Front right	99.9999 g
Maximum deviation from centric loading indication |ΔIcc| max = 0.0001 g	

Error of indication

Testload L	Indication I	Error E	Expansion factor k	Uncertainty $U(E)$	Uncertainty relative $U_{rel}(E)$
0.0100 g	0.0100 g	0.0000 g	2.00	0.00012 g	1.2 %
0.1000 g	0.1000 g	0.0000 g	2.00	0.00013 g	0.13 %
0.5000 g	0.5000 g	0.0000 g	2.00	0.00013 g	0.026 %
1.0000 g	1.0000 g	0.0000 g	2.00	0.00013 g	0.013 %
5.0000 g	5.0000 g	0.0000 g	2.00	0.00013 g	0.0026 %
10.0000 g	10.0000 g	0.0000 g	2.00	0.00013 g	0.0013 %
20.0000 g	20.0000 g	0.0000 g	2.00	0.00014 g	0.00068 %
50.0000 g	50.0000 g	0.0000 g	2.00	0.00019 g	0.00038 %
100.0000 g	100.0001 g	0.0001 g	2.00	0.00018 g	0.00018 %
200.0000 g	200.0000 g	0.0000 g	2.00	0.00026 g	0.00014 %
220.0000 g	220.0000 g	0.0000 g	2.00	0.00032 g	0.00015 %
Maximum error of indication		|E|max = 0.0001 g			

$U_{rel}(E)$ is the quotient of $U(E)$ and test load L. The uncertainty of measurement $U(E)$ is valid only if error E is considered. You will find reference notes on the uncertainty of measurement in use under: Appendix to the calibration certificate | Interpretation of measurement results.
Reference note: The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the documented Expansion factor, determined in accordance with the European Calibration Guideline EURAMET cg-18, V4.0. There is a 95 % probability that the value of the measurand will be in the assigned value range.

End of calibration certificate


Uncertainty of measurement in use

Device adjusted before measurement	Yes
Temperature deviation considered	1.5 K (isoCAL active)
Temperature coefficient considered	1 · 10⁻⁶/K
Uncertainty of the weighing result $U_{pi}(W)$	**$U_{pi}(W) = 0.00013\ g + 3.42 \cdot 10^{-4} \cdot R$**

Reference note: The current uncertainty of measurement is calculated by entering of the reading R into this formula. In relation to this, there is no need for a Expansion factor, because the reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied with an Expansion factor of 1, determined in accordance with the European Calibration Guideline EURAMET cg-18, V4.0. There is a 95 % probability that the value of the measurand will be in the assigned value range.

Indication in % from max load	Net indication R	Uncertainty $U_{pi}(W)$	Uncertainty relative $U_{pi}(W)_{rel}$
1 %	2.2000 g	0.00014 g	0.0063 %
25 %	55.0000 g	0.00032 g	0.00058 %
50 %	110.0000 g	0.00051 g	0.00046 %
75 %	165.0000 g	0.00069 g	0.00042 %
100 %	220.0000 g	0.00088 g	0.00040 %

Graphic realization of the relative uncertainty of measurement | process accuracy

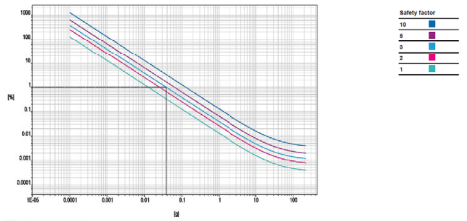

Displayed example

Process accuracy	1.00 %
Safety factor	3
Minimum sample weight	0.0380 g

SCG

Metrology

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110, Thailand.
Saraburi Tel : +66 3627 3096 Fax : +66 3627 3100
Bangkok Tel : +668 9205 6851 , +669 8247 2360
Website : www.scieco.co.th E-Mail : calibrate@scg.com

NSC-TISI-TIS 17025 CALIBRATION 0244

Certificate of Calibration

Equipment	:	Liquid Bath (Water)
Manufacturer	:	Memmert
Model	:	WNE29
Serial No.	:	L623.0105
Customer Code	:	RYG_EN0220
ID No.	:	T5650A5
Customer	:	ALS Laboratory Group (Thailand) Co.,Ltd. (Rayong Branch)
		616/10 Moo 5 T.Maenam Khu,
		A.Pluakdaeng, Rayong 21140
Customer Location	:	Wet Chemistry Lab
Date of Receipt	:	11 December 2024
Calibrated By	:	Atiphong Rongrat (Technician)
Approved By	:	/ Boonchai Suriyawong (Site Calibration Manager)
Date of Issue	:	20 DEC 2024

REVIEW BY Thanitak.
APPROVED BY
NEXT CAL DATE 19/12/25

The uncertainties are for a confidence probability of approximately 95%.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standard laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Metrology.

SCG

Metrology

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110, Thailand.

NSC-TISI-TIS 17025 CALIBRATION 0244

Calibration Report

Equipment	:	Liquid Bath (Water)
Date of Calibration	:	19 December 2024
Environment	:	Temperature : 25.3-25.9 °C
		Line Voltage : 221.4-225.4 V
		Relative Humidity : 55 - 65 %RH

Condition of this results of calibration :

1. This equipment was calibrated by insert five resistance thermometer detectors into its water bath , the other one thermocouple type T use for ambient temperature measurement . The calibration was done in according to WI-T36 (based on ASTM E715-80 (Reapproved 2001)).
   All data show below were final values and the initial data from customer request . The temperature scale used. was based on ITS - 90.
2. Reference standard instrument :

Instrument	Model	Instrument No.	Certificate No.	Due Date
RTD	100 OHM	M34 (CH1-CH5)	T240400	16 March 2025
DATA LOGGER	34970A	T193	T240400	16 March 2025

3. This certificate is traceable to :
   National Institute of Metrology (Thailand) through Metrological Center (NSC-TISI-TIS 17025 CALIBRATION 0244.)
4. Condition of calibrated item : good
   Equipment Description :
   Time Constar 1 Hour 30 Minute At 63 °C
5. Adjustment :
   (X) without adjustment ( ) after adjustment

Approved By.

SCG


Metrology

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110, Thailand.

NSC-TISI-TIS 17025 CALIBRATION 0244

Calibration Report

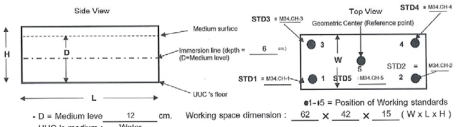

● 1~ ● 5 = Position of Working standards

- D = Medium leve 12 cm. Working space dimension : 62 × 42 × 15 (W x L x H)
- UUC 's medium : Water
- Working standards are located : 2.5 cm. away from each coner and walls.

Measurement Results:

Calibration Point	Average Standard Reading at each position (°C)				
	M34.CH-1	M34.CH-2	M34.CH-3	M34.CH-4	M34.CH-5
63	62.87	61.00	62.88	62.98	63.22
85	84.76	85.14	84.89	85.07	85.24

Liquid Bath (Water)			Temperature Distribution				
Setting (°C)	Reading (°C)		Average (°C)	Stability (±°C)	Uniformity (±°C)	Uncertainty (±°C)	Coverage Factor k
	Min , Max	Average					
63.0	-	63.0	62.99	0.07	0.25	0.23	2.00
85.0	-	85.0	85.02	0.13	0.35	0.28	2.00

The calibration result apply only the above calibrated item.
The result of test was found accurate as shown on date and place of test only.
The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor k which for a t-distribution, providing a level of confidence of approximately 95 % .

Approved By.

SCG

Metrology Center

SCI ECO Services Company Limited

51 Moo 8, Tubkwang, Kaeng Khoi, Saraburi, Thailand 18260
Bangkok Tel : +668 9205 6851 , +669 81924 0059
Saraburi Tel : +669 8247 2360
Website : www.scieco.co.th E-Mail : calibrate@scg.co.th

NSC-TISI-TIS 17025 CALIBRATION 0244

Certificate of Calibration

Equipment	:	**Liquid Bath (Water)**
Manufacturer	:	**Memmert**
Model	:	**WNE29**
Serial No.	:	**L623.0105**
Customer Code	:	**RYG_EN0220**
ID No.	:	**T5650A5**
Customer	:	**ALS Laboratory Group (Thailand) Co.,Ltd. (Rayong Branch)**
		616/10 Moo 5 T.Maenamkoo,
		A.Pluakdaeng, Rayong 21140
Customer Location	:	**Wet Chemistry Lab**
Date of Receipt	:	**19 November 2025**
Calibrated By	:	**Sujjar Naknakred (Site Calibration Manager)**
Approved By	:	**/ Boonchai Suriyawong (Site Calibration Manager)**
Date of Issue	:	01 DEC 2025

REVIEW BY Thanitak.
APPROVED BY
NEXT CAL DATE 27/11/26

The uncertainties are for a confidence probability of approximately 95%.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standard laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Metrological Center.

SCG

Metrology Center

SCI ECO Services Company Limited

51 Moo 8, Tubkwang, Kaeng Khoi, Saraburi, Thailand 18260

NSC-TISI-TIS 17025 CALIBRATION 0244

Calibration Report

Equipment	:	**Liquid Bath (Water)**
Date of Calibration	:	**27 November 2025**
Environment	:	**Temperature : 25.5-25.7 °C**
		Line Voltage : 221.8-225.5 V
		Relative Humidity : 55 - 65 %RH

Condition of this results of calibration :

1. This equipment was calibrated by insert five resistance thermometer detectors into its water bath , the other one thermocouple type T use for ambient temperature measurement . The calibration was done in according to WI-T36 (based on ASTM E715-80 (Reapproved 2022)).
   All data show below were final values and the initial data from customer request . The temperature scale used was based on ITS - 90 .
2. Reference Standard Instrument :

Instrument	Model	Instrument No.	Certificate No.	Due Date
RTD	100 OHM	M18 (CH1-CH5)	T251758	17 October 2026
DATA LOGGER	34970A	T261	T251758	17 October 2026

3. This certificate is traceable to :
   National Institute of Metrology (Thailand) through Metrological Center (NSC-TISI-TIS 17025 CALIBRATION 0244.)
4. Condition of calibrated item : good
   Equipment Description :
   Time Constant 1 Hour 3 Minute At 63 °C
5. Adjustment :
   (X) without adjustment ( ) after adjustment

Approved By.

SCG


Metrology Center

SCI ECO Services Company Limited

51 Moo 8, Tubkwang, Kaeng Khoi, Saraburi, Thailand 18260

NSC-TISI-TIS 17025 CALIBRATION 0244

Calibration Report



● 1~ ● 5 = Position of Working standards

- D = Medium level : 12 cm. Working space dimension : 59 × 35 × 14 (WxLxH)
- UUC 's medium : Water
- Working standards are located at 2.5 cm. away from each coner and walls.

Measurement Results:

Calibration Point	Average Standard Reading at each position (°C)				
	CH-1	CH-2	CH-3	CH-4	CH-5
63	62.93	63.13	62.94	63.10	63.09
85	85.15	85.33	85.21	85.43	85.20

Liquid Bath (Water)			Temperature Distribution				
Setting (°C)	Reading (°C)		Average (°C)	Stability (±°C)	Uniformity (±°C)	Uncertainty (±°C)	Coverage Factor k
	Min , Max	Average					
63.0	62.9 , 63.1	63.0	63.04	0.08	0.17	0.27	2.06
85.0	84.8 , 85.2	85.0	85.26	0.13	0.24	0.43	2.23

*** The quoted uncertainty exclude "uniformity"**
The calibration result apply only the above calibrated item.
The result of test was found accurate as shown on date and place of test only.
The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor k which for a t-distribution, providing a level of confidence of approximately 95 % .

End of Certificate.

Approved By.

DKSH

Certificate of Calibration

Equipment:	SPECTROPHOTOMETER	Certificate No.:	C06250108
Model:	DR6000	Issued Date:	18 March 2025
Serial No. (s ID.):	1027840 (RYG_EN0037)	Job No.:	WO-00064379
Manufacturer:	HACH	Page:	1 of 3
Condition:	In Condition		

Customer: ALS Laboratory Group (Thailand) Co.,Ltd. (Rayong Branch)
616/10 Moo 5 T.Maenam Khu,
A.Pluakdaeng, Rayong 21140, Thailand.

Received by : Photchanan.
APPROVED BY
NEXT CAL. DATE 18/09/26

Environment Condition: Temperature 24.4 °C ± 0.3 °C
Humidity 60.8 %RH ± 3.5 %RH

Calibration Place: ALS Laboratory Group (Thailand) Co.,Ltd. (Rayong Branch)
(Wet Chemistry Lab)
616/10 Moo 5 T.Maenam Khu, A.Pluakdaeng, Rayong 21140, Thailand.

Calibration By: Mr.Preecha Phooarsai
Calibration Date: 18 March 2025
The Method used: In house method, CAL-WI-2I, base on ASTM E 275-08 and ASTM E 387-04
Traceability: This certificate is traceable to the CRM maintained by National Institute of Standards and Technology (NIST) through Starna Scientific Limited.
The standard for Wavelength Certificate No. 111583 and 111584
The standard for Photometric Certificate No. 9114984 and 111588
The standard for Stray light Certificate No. 111586 and 111585
The standard for Spectral resolution Certificate No. 111587

(Mr. Preecha Phooarsai)
Person in charge

(Miss Kaewkan Suradech)
Authorized signatory

This certificate is issued the units of measurement according to the International System of Units (SI). It provides traceability of measurement to international or national standard or other recognized national standard laboratories.
The measurement uncertainty stated is the expanded uncertainty which is obtained from the standard uncertainty multiplied by the coverage factor (k=2) to provide a level of confidence of approximately 95%. It is determined in accordance with the Guide to Expression of Uncertainty in Measurement (GUM).
These results may be affected by deviations from specified conditions. The results relate only to the items tested, calibrated or sampled. The report shall not be reproduced except in full without approval of DKSH Technology Limited.

บริษัท ดีเคแซกเซอร บจก/DKSH Technology Limited
DKSH Technology Limited
2533 ถนนสุขุมวิท แขวงพระโขนง เขตพระโขนง กรุงเทพมหานคร 10260
2533 Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Phone: +66 2639 7000 Email: info.calibration@dksh.com Website: www.dksh.com/scientific-thailand

Calibration Results:
Without Adjustment

Wavelength Accuracy (nm), The spectral bandwidth of Std at 2 nm and UUC at 2 nm

Standard Wavelength	Unit Under Calibration	Correction	Uncertainty
418.61	418.5	0.11	0.13
536.66	536.7	-0.04	0.13
637.98	638.3	-0.32	0.13
748.48	748.8	-0.32	0.13
807.03	807.5	-0.47	0.13

Photometric Accuracy (Absorbance)

Wavelength	Standard absorbance	Unit Under Calibration	Correction	Uncertainty
420 nm	0.0000	0.000	0.0000	0.0045
	0.2930	0.291	0.0020	0.0045
	0.5168	0.518	-0.0012	0.0045
	1.0298	1.031	-0.0012	0.0045
440 nm	0.0000	0.000	0.0000	0.0045
	0.2867	0.285	0.0017	0.0045
	0.5073	0.508	-0.0007	0.0045
	1.0083	1.009	-0.0007	0.0045
465 nm	0.0000	0.000	0.0000	0.0045
	0.2516	0.250	0.0016	0.0045
	0.4595	0.461	-0.0015	0.0045
	0.9334	0.935	-0.0016	0.0045
546.1 nm	0.0000	0.000	0.0000	0.0045
	0.2461	0.246	0.0001	0.0045
	0.4652	0.466	-0.0008	0.0045
	0.9468	0.948	-0.0012	0.0045
590 nm	0.0000	0.000	0.0000	0.0045
	0.2594	0.259	0.0004	0.0045
	0.5040	0.505	-0.0010	0.0045
	1.0032	1.004	-0.0008	0.0045
635 nm	0.0000	0.000	0.0000	0.0045
	0.2579	0.258	-0.0001	0.0045
	0.4971	0.497	0.0001	0.0045
	0.9720	0.973	-0.0010	0.0045

บริษัท ดีเคแซกเซอร บจก/DKSH Technology Limited
DKSH Technology Limited
2533 ถนนสุขุมวิท แขวงพระโขนง เขตพระโขนง กรุงเทพมหานคร 10260
2533 Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Phone: +66 2639 7000 Email: info.calibration@dksh.com Website: www.dksh.com/scientific-thailand
Delivering Growth – in Asia and Beyond.
CAL-FM-C06-16: 11 Mar 2024

Calibration Results:
Without Adjustment

Photometric Accuracy (Absorbance)

Wavelength	Standard absorbance	Unit Under Calibration	Correction	Uncertainty
235 nm	0.0000	0.000	0.0000	0.0080
	0.7355	0.738	-0.0025	0.0080
257 nm	0.0000	0.000	0.0000	0.0080
	0.8574	0.857	0.0004	0.0080
313 nm	0.0000	0.000	0.0000	0.0080
	0.2864	0.290	-0.0036	0.0080
350 nm	0.0000	0.000	0.0000	0.0080
	0.6374	0.637	0.0004	0.0080

Stray light *

Standard: cut-off	UUC: Wavelength (nm)	UUC: Transmission (%T)	Absorbance (A)
260.62 +/- 0.11 nm	260.6	1.7	1.770
391.44 +/- 0.11 nm	391.4	1.4	1.854

Spectral Resolution *

Nominal Concentration 0.02 % v/v	Peak	Trough	Ratio	SBW
Standard Wavelength (nm)	268.66	266.69	1.38	2.00
UUC: Wavelength (nm)	268.2	266.2		
Std Absorbance (A)	0.4566	0.2780		
UUC: Absorbance (A)	0.413	0.299		

* Calibration Marked " Not TISI Accredited " in this Certificate have been included for completeness.

The End of Certificate

บริษัท ดีเคแซกเซอร บจก/DKSH Technology Limited
DKSH Technology Limited
2533 ถนนสุขุมวิท แขวงพระโขนง เขตพระโขนง กรุงเทพมหานคร 10260
2533 Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Phone: +66 2639 7000 Email: info.calibration@dksh.com Website: www.dksh.com/scientific-thailand
Delivering Growth – in Asia and Beyond.
CAL-FM-C06-16: 11 Mar 2024

DKSH

ใบตรวจสอบสภาพเครื่องวัดสิ่งแวดล้อม

เลขที่ใบงาน: WO-00064379

ชนิดเครื่องมือ: SPECTROPHOTOMETER รุ่น: DR6000 หมายเลขเครื่อง: 1627845

ตรวจสอบ (วัน) 18 Mar 2025 ปกติ	ไม่ปกติ	รายการตรวจเช็ค	ตรวจสอบ (ผล) 18 Mar 2025 ปกติ	ไม่ปกติ	หมายเหตุ
		General			
☑	☐	1. ความสมบูรณ์เครื่อง	☑	☐	
☑	☐	2. ความสะอาด (ของใส่ตัวอย่าง, ภายใน-นอกเครื่อง)	☑	☐	
☑	☐	3. สวิทช์ ปิด – เปิด เครื่อง (On-Off Swicth)	☑	☐	
☑	☐	4. ปุ่มกด (Keypad)	☑	☐	
☑	☐	5. หน้าจอ (Display, Screen Contrast)	☑	☐	
		Spectrophotometer			
☐	☐	6. แรงดันไฟฟ้า (Battery Backup) >= 2.5 VDC	☐	☐	
☐	☐	7. ตัวหมุนเลือกความยาวคลื่น (Wavelength Control)	☐	☐	
☑	☐	8. ความยาวคลื่น (Wavelength Chack)	☑	☐	*
☑	☐	9. แหล่งกำเนิดแสง (UV < 3,000 hour)	☑	☐	13.5 Hours
☑	☐	10. แหล่งกำเนิดแสง (Visible < 5,000 hour)	☑	☐	893.0 Hours
☑	☐	11. ช่องวัดหลายตัวอย่าง (Carousel Module)	☑	☐	
		pH Meter and Conductivity Meter			
☐	☐	12. อิเล็คโทรด (Electrode and Connection Cable)	☐	☐	
☐	☐	13. ระดับสารละลายใน Electrode (Level KCl)	☐	☐	
☐	☐	14. ฝาปิดกันเปลาย Electrode (Dust Protection Hood)	☐	☐	
☐	☐	15. ขาจับอิเล็คโทรด (Stand)	☐	☐	
		Turbidimeter			
☐	☐	16. ค่าความขุ่นที่ต่ำสุด (No Sample)	☐	☐	
☐	☐	17. ระดับการต้องล้างของแสง (>= 2.5 ไม่เกิน 3.0)	☐	☐	
		Automatic titrator			
☐	☐	18. สภาพ Piston Burettes	☐	☐	
☐	☐	19. Function Rinsing and Dosing	☐	☐	
☐	☐	20. ระบบท่อสายยางและอุปกรณ์ประกอบ	☐	☐	

เพิ่มเติมข้อแนะนำ : * 656.1nm = 656.1nm
* 486.0nm = 485.7nm

Mr.Preecha Phooarsai
Service Engineer

บริษัท ดีเคแซกเซอร บจก/DKSH Technology Limited
DKSH Technology Limited
2533 ถนนสุขุมวิท แขวงพระโขนง เขตพระโขนง กรุงเทพมหานคร 10260
2533 Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Phone: +66 2639 7000 Email: info.calibration@dksh.com Website: www.dksh.com/scientific-thailand

TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL.0-2717-3000-29 FAX.0-2719-9484

NSC-TISI-TIS17025 CALIBRATION 0008

Certificate of Calibration

Cert.No.: 25CH1001
Page.: 1 of 3

Equipment :	pH Meter
Manufacturer :	Mettler Toledo
Model :	Seven2Go S2
Serial No. :	C232588424
ID No. :	RYG_FS0605
Condition As-Received:	Used Item
Received Date :	22 August 2025
Calibration Date :	25 August 2025
Reference :	2508-0746DSC-1
Submitted by :	ALS Laboratory Group (Thailand) Co.,Ltd. Rayong Branch 616/10 Moo 5, T.Maenam Khu, A.Pluakdaeng, Rayong 21140, Thailand
Ambient Temperature :	(25 ± 2.5) °C
Relative Humidity :	(50 ± 15) %
Calibration Procedure :	In - house method : - CP-CH5 by direct measurement with DC voltage standard and direct measurement with certified reference material (CRM) - CP-CH8 by comparison with temperature standard
Calibrated by :	Walalak Sirithean
Approved by :	Saithip Approved Signatory
	( ) Chakrit Waewwanjua
	( ) Ponpan Paipim
	(√) Saithip Meangmai
Issue Date :	26 August 2025

REVIEW BY Pitthaya T.
APPROVED BY S.S.
NEXT CAL DATE 25/08/26

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

Condition of this calibration result

1. Reference Standard Instrument

Instrument	Serial No.	ID No.	Cert. No.	Due Date
1) Document Process Calibrator	58440003	130RC120	24E3731	25 Nov 2025
2) Ref. Standard Thermometer	49850S4	110RC044	25I708	03 July 2026

- This measurement result is traceable to SI throught Technology Promotion Association (Thailand - Japan)

2. Certified Reference Materials : The measurement results are traceable to SI through CPA chem Ltd., ANSI-ASQ National Accreditation Board, Accredited No. AR-1835

Buffer Solution	Manufacturer	Lot No.	Exp. date
pH 4.007	CPA chem	1066665	18 Jan 2027
pH 6.987	CPA chem	1034204	27 Sep 2025
pH 10.010	CPA chem	1114385	08 June 2026

3. This certificate is valid only to the item calibrated on date and place of calibration.

Calibration Results
Function : mV Measurement
Performing standard curve by Document Process Calibrator at pH (4,7,10)

Unit Under Calibration	Nominal Value	Standard Voltage Input	Actual Reading		Uncertainty of Measurement (±mV)	Coverage factor k
	pH	mV	mV	pH		
pH Meter	4.00	177.48	178	4.00	0.58	2.00
S/N.: C232588424	7.00	0.00	0	7.00	0.58	2.00
	10.00	-177.48	-177	10.00	0.58	2.00

Calibration Results
Function : pH Measurement
Performing three buffers standard curve by using buffer nominal pH (4,7,10)

Unit Under Calibration	Standard pH Buffer Solution	Actual pH Reading	Actual mV Reading (mV)	Uncertainty of pH Measurement (±)	Coverage factor k
pH Electrode	4.007	4.00	149	0.0071	2.00
S/N.: 2465869	6.987	7.01	-26	0.0086	2.00
	10.010	10.01	-195	0.0092	2.00

Function : Temperature Measurement
(*) Without adjustment
This equipment was connected with Temperature Probe;
- Model : InLab Expert Go-ISM
- Serial No. : 2465869
Dimension of probe
- Length : 120 mm.
- Diameter : 12 mm.
- Immersion Depth : 100 mm.

Calibration Point (°C)	Standard Temperature (°C)	UUC* Reading (°C)	Error (°C)	Uncertainty of measurement (± °C)	Coverage factor k
25.0	25.001	25.3	0.299	0.13	2.00
45.0	45.001	45.4	0.399	0.13	2.00

Remark - UUC* = Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-end-

SCG

Metrology
SCI ECO Services Company Limited
33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110, Thailand.
Saraburi Tel : +66 3627 3096 Fax : +66 3627 3100
Bangkok Tel : +668 9205 6851 , +669 8247 2360
Website : www.scieco.co.th E-Mail : calibrate@scg.com

NSC-TISI-TIS 17025 CALIBRATION 0244

Certificate No. T241120 Page 1 of 4

Certificate of Calibration

Equipment	:	**Chamber (Cold Room)**
Manufacturer	:	**MODULAR**
Model	:	**IREVCOHCOO**
Serial No.	:	**C00351459**
Customer Code	:	**RYG_EN0184**
ID No.	:	**T1939A5**
Customer	:	**ALS Laboratory Group (Thailand) Co.,Ltd. (Rayong Branch)**
		616/10 Moo 5 T.Maenam Khu,
		A.Pluakdaeng, Rayong 21140
Customer Location	:	**Laboratory**
Date of Receipt	:	**5 June 2024**
Calibrated By	:	**Sujjar Naknakred (Site Calibration Manager)**
Approved By	:	**Preecha Phisassutthikul (Temperature Calibration Manager)**
Date of Issue	:	12 JUN 2024

REVIEW BY Thanitall.
APPROVED BY
NEXT CAL. DATE 11/12/25

The uncertainties are for a confidence probability of approximately 95%.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standard laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Metrology.

SCG

Metrology
SCI ECO Services Company Limited
33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110, Thailand.

NSC-TISI-TIS 17025 CALIBRATION 0244

Calibration Report

Equipment	:	**Chamber (Cold Room)**
Date of Calibration	:	**11 June 2024**
Environment	:	**Temperature : 23.1-24.1 °C**
		Line Voltage : 222.3-226.3 V
		Relative Humidity : 55 - 65 %RH

Condition of this results of calibration :

1. This equipment was calibrated by insert nine standard thermocouples type T into its chamber , the other one standard thermocouples type T use for ambient temperature measurement . The calibration was done in according to WI-T20 (based on ASTM E145-94 (Reapproved 2001) and AS2853-1986).
All data show below were final values and the initial data from customer request . The temperature scale used was based on ITS - 90 .
2. Reference Standard Instrument :


Instrument	Model	Instrument No.	Certificate No.	Due Date
TC	TYPE T	TN161-TN170	T240713	19 April 2025
TC	TYPE T	TN171-TN180	T240713	19 April 2025
DATA LOGGER	34970A	T149	T240713	19 April 2025

3. This certificate is traceable to :
National Institute of Metrology (Thailand) through Metrological Center (NSC-TISI-TIS 17025 CALIBRATION 0244.)
4. Condition of calibrated item : good
Equipment Description :
Time Constant 3 Hour 30 Minute At 3 °C
Fresh Air Damper ☐ Open ☐ Min ☐ Medium ☐ Max
☐ Close
☒ Not Available
5. Adjustment :
( ) without adjustment (X) after adjustment

Approved By

Certificate No. T241120 Page 3 of 4

Calibration Report



C = Centre , F = Centre of Face , A = Corner , E = Centre of Edge

1C	=	TN161	11F	=	TN171
2A	=	TN162	12F	=	TN172
3A	=	TN163	13A	=	TN173
4F	=	TN164	14A	=	TN174
5A	=	TN165	15F	=	TN175
6A	=	TN166	16E	=	TN176
7F	=	TN167			
8F	=	TN168			
9A	=	TN169			
10A	=	TN170			

Approved By.

Certificate No. T241120 Page 4 of 4

Calibration Report

Measurement Results:

Calibration Point	Average Standard Reading at each position (°C)								
	TN161	TN162	TN163	TN164	TN165	TN166	TN167	TN168	TN169	TN170
3	2.73	2.70	2.77	2.79	2.99	2.35	3.09	3.21	3.08	2.90
	TN171	TN172	TN173	TN174	TN175	TN176				
	3.39	3.01	2.92	2.81	3.42	3.42				

Chamber (Cold Room)			Temperature Distribution				
Setting (°C)	Reading (°C)		Average (°C)	Stability (±°C)	Uniformity (°C)	Uncertainty (±°C)	Coverage Factor *k*
	Min , Max	Average					
3.0	2.9 , 4.4	3.7	2.97	1.32	1.13	2.02	2.00

* The quoted uncertainty exclude " uniformity "
The calibration result apply only the above calibrated item.
The result of test was found accurate as shown on date and place of test only.
The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor *k* which for a t-distribution, providing a level of confidence of approximately 95 % .

Approved By.

Certificate No. T252167 Page 1 of 4

Certificate of Calibration

Equipment	:	**Chamber (Cold Room)**
Manufacturer	:	**MODULAR**
Model	:	**IREVCOHCOO**
Serial No.	:	**C00351459**
Customer Code	:	**RYG_EN0184**
ID No.	:	**T1939A5**
Customer	:	**ALS Laboratory Group (Thailand) Co.,Ltd. (Rayong Branch)**
		616/10 Moo 5 T.Maenamkoo,
		A.Pluakdaeng, Rayong 21140
Customer Location	:	**ENVIRONMENT LABORATORY**
Date of Receipt	:	**19 November 2025**
Calibrated By	:	**Sujjar Naknakred (Site Calibration Manager)**
Approved By	:	**/ Boonchai Suriyawong (Site Calibration Manager)**
Date of Issue	:	01 DEC 2025

REVIEW BY Thanitall
APPROVED BY
NEXT CAL. DATE 27/05/27

The uncertainties are for a confidence probability of approximately 95%.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standard laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Metrological Center.

Certificate No. T252167 Page 2 of 4

Calibration Report

Equipment	:	**Chamber (Cold Room)**
Date of Calibration	:	**27 November 2025**
Environment	:	**Temperature : 24.7-25.6 °C**
		Line Voltage : 222.3-226.3 V
		Relative Humidity : 55 - 65 %RH

Condition of this results of calibration :

1. This equipment was calibrated by insert nine standard themocouples type T into its chamber , the other one standard thermocouples type T use for ambient temperature measurement . The calibration was done in according to WI-T20 (based on ASTM E145-94 (Reapproved 2019) and AS2853-1986).
   All data show below were final values and the initial data from customer request . The temperature scale used was based on ITS - 90 .
2. Reference Standard Instrument .


Instrument	Model	Instrument No.	Certificate No.	Due Date
TC	TYPE T	TN161-TN170	T251760	17 October 2026
TC	TYPE T	TN171-TN180	T251760	17 October 2026
DATA LOGGER	34970A	T261	T251760	17 October 2026

3. This certificate is traceable to :
   National Institute of Metrology (Thailand) through Metrological Center (NSC-TISI-TIS 17025 CALIBRATION 0244.)
4. Condition of calibrated item : good
   Equipment Description :
   Time Constant 1 Hour 12 Minute At 3 °C
   Fresh Air Damper ☐ Open ☐ Min ☐ Medium ☐ Max
   ☐ Close
   ☒ Not Available
5. Adjustment :
   ( ) without adjustment (X) after adjustment

Approved By.

Certificate No. T252167 Page 3 of 4

Calibration Report

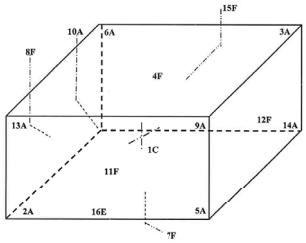

C = Centre , F = Centre of Face , A = Comer , E = Centre of Edge

1C	=	TN161	11F	=	TN171
2A	=	TN162	12F	=	TN172
3A	=	TN163	13A	=	TN173
4F	=	TN164	14A	=	TN174
5A	=	TN165	15F	=	TN175
6A	=	TN166	16E	=	TN176
7F	=	TN167			
8F	=	TN168			
9A	=	TN169			
10A	=	TN170			

Approved By.

Certificate No. T252167 Page 4 of 4

Calibration Report

Measurement Results:

Calibration Point	Average Standard Reading at each position (°C)									
	1C TN161	2A TN162	3A TN163	4F TN164	5A TN165	6A TN166	7F TN167	8F TN168	9A TN169	10A TN170
3	2.59	2.80	2.94	2.86	3.05	3.44	3.11	3.30	3.29	3.66
	11F TN171	12F TN172	13A TN173	14A TN174	15F TN175	16E TN176				
	3.41	3.56	3.38	3.54	3.36	3.16				

Chamber (Cold Room)			Temperature Distribution				
Setting (°C)	Reading (°C)		Average (°C)	Stability(±°C)	Uniformity(°C)	Uncertainty(±°C)	Coverage Factor *k*
	Min , Max	Average					
3.0	2.9 , 4.1	3.7	3.21	1.25	1.92	1.85	2.00

* The quoted uncertainty exclude " uniformity "
The calibration result apply only the above calibrated item.
The result of test was found accurate as shown on date and place of test only.
The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor *k* which for a t-distribution, providing a level of confidence of approximately 95 % .

End of Certificate.

Approved By.

© 2024 by Agilent Technologies Agilent CrossLab Compliance Services

Certificate of System Qualification

GC-OQ + GCMS-OQ

System ID: BKK_EN0259(GM-7)
Organization Name: ALS Laboratory Group (Thailand) Co., Ltd.
Organization Location: 104 Patthanakarn 40, Patthanakarn Rd., Khwang Suan Luang, Khet Suan Luang, Bangkok
Date: June 25, 2025 8:40:18 PM
EQP Name: AgilentRecommended , AgilentRecommended
EQP Revision: GC.02.50, GCMS.02.50
Overall Qualification Status: Pass

REVIEW BY Mint Sut
APPROVED BY
NEXT CAL. DATE 25-Dec-26

System Inspection and Basic Safety and Operation

Name: 7890
Setpoint Status: Pass

Overall System Inspection and Basic Safety and Operation Test Status: Pass

Inlet Pressure Accuracy

Name: 7890 Front SSL
Setpoint Status: Pass

	Setpoint	Actual	
Inlet Pressure:	25.0 psi	25.2 psi	
Accuracy:		0.2	psi
Agilent Recommended:		<= 1.2	

Overall Inlet Pressure Accuracy Test Status: Pass

GC Oven Temperature Accuracy

© 2024 by Agilent Technologies Agilent CrossLab Compliance Services

Name: 7890
Setpoint Status: Pass
Zone: Oven

	Setpoint	Actual	
Temperature:	230.0	229.8	°C
Accuracy:		-1.2	°C
Agilent Recommended:	>= -1.0	% setpoint in K	(-5.0 °C)
	<= 1.0	% setpoint in K	(5.0 °C)

Setpoint Status: Pass
Zone: Oven

	Setpoint	Actual	
Temperature:	100.0	100.8	°C
Accuracy:		0.8	°C
Agilent Recommended:	>= -1.0	% setpoint in K	(-3.7 °C)
	<= 1.0	% setpoint in K	(3.7 °C)

Overall GC Oven Temperature Accuracy Test Status: Pass

GC Oven Temperature Stability

Name: 7890
Setpoint Status: Pass

	Setpoint	Average	
Temperature:	100.0	101.0	°C
Stability:		0.0	°C
Agilent Recommended:	<=	0.5	

Overall GC Oven Temperature Stability Test Status: Pass

Log Amp

Tested Combination1 Front SSL / External SQ
Name: 5977A

© 2024 by Agilent Technologies Agilent CrossLab Compliance Services

Setpoint Status: Pass

Overall Log Amp Test Status: Pass

RFPA

Tested Combination1 Front SSL / External SQ
Name: 5977A
Setpoint Status: Pass

Amu:	1050 m/z	Drift After Five Minutes:	2 mV		RFPA Voltage:	462 mV
Agilent Recommended:	>= -100	and	<= 100		<= 1100	

Overall RFPA Test Status: Pass

Tune EI

Tested Combination1 Front GSL / External SQ
Name: 5977A
Setpoint Status: Pass
Filament: 1
Setpoint Status: Pass
Filament: 2

Overall Tune EI Test Status: Pass

Signal to Noise EI

Tested Combination1 Front SSL / External SQ
Name: 5977A

Source:	EI - Extractor	Filament:	1
Setpoint Status:	Pass		
Signal to Noise:	35794093955		
Agilent Recommended:	>=	1200	
Source:	EI - Extractor	Filament:	2
Setpoint Status:	Pass		
Signal to Noise:	3289496829		
Agilent Recommended:	>=	1200	

Overall Signal to Noise EI Test Status

Pass

NOTE: This test's 0 comment(s) and 3 deviation(s) are available in the Attachments section.

Instrument Details

Purpose

This section describes the as found system configuration.

Details

System

System ID	BKK_EN0259(GM-7)
Manufacturer	Agilent Technologies
Name	7890

Tested Combination1

Injection Technique	Manual Injection
Inlet	Front
Detector	External
LTM Included?	No

Sampler 1

Manufacturer	Agilent Technologies
Type	Manual Injection
Usage	Sample Injection
Syringe Volume (µL)	10

Mainframe 1

Manufacturer	Agilent Technologies
Name	7890
Model Number	G3442B
Serial Number	CN14133181
Firmware Revision	B.02.03
Oven Type	Standard

Inlet 1

Manufacturer	Agilent Technologies
Name	7890
Type	SSL
Location	Front
Carrier Gas	Helium
Control Type	Electronic Pressure Control (EPC)
Purged Inlet	Yes

Detector 1

Manufacturer	Agilent Technologies
Name	Mass Spectrometer
Type	Mass Spectrometer
Location	External

Mass Spectrometer 1

Manufacturer	Agilent Technologies
Type	SQ
Name	5977A
Serial Number	US1415M209
Firmware Revision	5977 6.00.21
High Vacuum System	Turbo Pump
Scouting Run Standard	OFN Std

MS EI Source 1

Manufacturer	Agilent Technologies
Source Type	EI - Extractor
Number of filaments	2

Electronic Signature

Purpose

This signature page was created and published because the ACE sign-off action was executed, which is valid for the entire document, including attachments. The ACE sign-off is an electronic signature that requires two distinct identification components: unique username and personal password. The Agilent representative who has delivered this service understands the meaning and legal status of an electronic signature. As a trained official operator, the Agilent representative has a unique password and logon to access ACE and electronically sign this document. (Other e-signatures can be applied to this document using a Document Content Management or other suitable method defined in your data access and control procedures.)

Details

Full Name of Signer:	Supasak Nimsongtham
Logged On User Name:	supasak.nimsongtham@agilent.com
Signature Creation Date:	June 25, 2025
Reason for Signature:	Executed protocol and published this original version of document

ACE Self Qualification Status

The installed version of ACE used to deliver this service passed qualification; the results conform with expected values. The self qualification summary report is available in the session folder location [C:\Qual\ace6\qual\ace6selfqualification.

Regulatory Disclaimer

This document provides a protocol to verify and record instrument configuration and evidence of proper operation. It has been prepared from our interpretation of applicable regulations as well as industry best practices. The document is designed to provide an important component of a complete compliance package. Validation depends upon many factors and use of this protocol alone does not assure compliance. Agilent Technologies makes no promises or representations as to its sufficiency for any specific regulatory program.

Warranty

Agilent Technologies makes no warranty of any kind to this material, including but not limited to, the implied warranties or merchantability and fitness for a particular purpose. Agilent Technologies shall not be liable for errors contained herein or for incidental or consequential damages in connection with the furnishing, performance, or use of this material.

User Name: supasak.nimsongtham
Report Generated by Hostname: SCG1115HKC

System Id: BKK_EN0259(GM-7)
Print Date: June 25, 2025 8:40:20 PM

GM-7-2025 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
June 13, 2025 10:01:23 AM	Audit	SessionCreated	Session	Host Name: SCG1115HKC, Drive Serial Number: C2031778
June 13, 2025 10:01:24 AM	start	Configuration	Session	None
June 13, 2025 10:01:24 AM	Audit	Entitlement	Licensing	User is FieldEngineer and does not require an unlock code
June 13, 2025 10:04:40 AM	Audit	EspLoaded	Session	EQP details for primary technique [Dc] - File path: [ProtocolPacks/Dc/Configurations/02.00/Dc.02.00.eqp], EQP File Name: [Dc.02.00.eqp], EQP Name: [AgilentRecommended],Protocol Revision :[Dc.02.50] EQP details for hyphenated technique [Dc/Ms] - File path: [ProtocolPacks/Gc/Ms/Configurations/02.00/Gc.Ms.02.50.eqp], EQP File Name: [Gc.Ms.02.50.eqp], EQP Name: [AgilentRecommended]
June 13, 2025 10:04:51 AM	End	Configuration	Session	None
June 13, 2025 10:05:03 AM	start	Qualification	Session	OQ
June 13, 2025 10:05:08 AM	start	Execution	System Inspection and Basic Safety and Operation - 7890 - Qualitative Test - No setpoints associated	None
June 13, 2025 10:06:35 AM	End	Execution	System Inspection and Basic Safety and Operation - 7890 - Qualitative Test - No setpoints associated	Run Count : 1

User Name: supasak.nimsongtham
Report Generated by Hostname: SCG1115HKC

System Id: BKK_EN0259(GM-7)
Print Date: June 25, 2025 8:40:20 PM

GM-7-2025 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
June 13, 2025 10:06:40 AM	start	Execution	Inlet Pressure Accuracy - Front SSL - Pressure Controlled Inlet - S: 25.0 psi - L: <= 1.2 psi AND <= 1.0 % setpoint in K	None
June 13, 2025 10:06:58 AM	End	Execution	Inlet Pressure Accuracy - Front SSL - Pressure Controlled Inlet - S: 25.0 psi - L: <= 1.2 psi	Run Count : 1
June 13, 2025 10:07:00 AM	start	Execution	GC Oven Temperature Accuracy - 7890 - Temperature : Oven - S: 230.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	None
June 13, 2025 10:07:30 AM	Audit	Data	GC Oven Temperature Accuracy - 7890 - Temperature : Oven - S: 230.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	Manual Data Entry
June 13, 2025 10:07:35 AM	End	Execution	GC Oven Temperature Accuracy - 7890 - Temperature : Oven - S: 230.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	Run Count : 1
June 13, 2025 10:07:59 AM	start	Execution	RFPA - 5977A SQ - Source: EI - Extractor	None
June 13, 2025 10:11:14 AM	start	Execution	GC Oven Temperature Accuracy - 7890 - Temperature : Oven - S: 100.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	None
June 13, 2025 10:12:12 AM	Audit	Data	GC Oven Temperature Accuracy - 7890 - Temperature : Oven - S: 100.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	Manual Data Entry
June 13, 2025 10:12:17 AM	End	Execution	GC Oven Temperature Accuracy - 7890 - Temperature : Oven - S: 100.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	Run Count : 1

User Name: supasak.nimsongtham
Report Generated by Hostname: SCG1115HKC

System Id: BKK_EN0259(GM-7)
Print Date: June 25, 2025 8:40:20 PM

GM-7-2025 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
June 13, 2025 10:12:19 AM	start	Execution	GC Oven Temperature Stability - 7890 - Temperature : Oven - S: 100.0°C - L: <= 0.5°C	None
June 13, 2025 10:30:39 AM	Audit	Data	GC Oven Temperature Stability - 7890 - Temperature : Oven - S: 100.0°C - L: <= 0.5°C	Manual Data Entry
June 13, 2025 10:30:45 AM	End	Execution	GC Oven Temperature Stability - 7890 - Temperature : Oven - S: 100.0°C - L: <= 0.5°C	Run Count : 1
June 13, 2025 10:30:56 AM	start	Execution	Log Amp - 5977A SQ - Source: EI - Extractor	None
June 13, 2025 10:31:15 AM	End	Execution	Log Amp - 5977A SQ - Source: EI - Extractor	Run Count : 1
June 13, 2025 10:34:14 AM	Audit	AceClosed	Session	None
June 16, 2025 11:55:53 AM	Audit	AceRestarted	Session	Host Name: DESKTOP-6PKI2AL, Drive Serial Number: 9456EA83
June 16, 2025 11:55:55 AM	Audit	SessionReloaded	Session	None
June 16, 2025 11:56:07 AM	start	Qualification	Session	OQ
June 16, 2025 5:47:31 PM	Audit	AceClosed	Session	None
June 17, 2025 1:34:47 PM	Audit	AceRestarted	Session	Host Name: DESKTOP-6PKI2AL, Drive Serial Number: 949AEA83
June 17, 2025 1:39:58 PM	Audit	AceClosed	Session	None
June 17, 2025 1:52:55 PM	Audit	AceRestarted	Session	Host Name: DESKTOP-6PKI2AL, Drive Serial Number: 949AEA83
June 17, 2025 2:03:56 PM	Audit	SessionReloaded	Session	None
June 17, 2025 2:03:56 PM	start	Qualification	Session	OQ
June 17, 2025 2:04:08 PM	Audit	AceClosed	Session	None

User Name: supasak.nimsongtham
Report Generated by Hostname: SCG1115HKC

System Id: BKK_EN0259(GM-7)
Print Date: June 25, 2025 8:40:20 PM

GM-7-2025 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
June 25, 2025 3:07:51 PM	Audit	AceRestarted	Session	Host Name: SCG1115HKC, Drive Serial Number: C2031778
June 25, 2025 3:07:54 PM	Audit	SessionReloaded	Session	None
June 25, 2025 3:09:13 PM	start	Qualification	Session	OQ
June 25, 2025 3:09:36 PM	start	Execution	RFPA - 5977A SQ - Source: EI - Extractor	None
June 25, 2025 3:10:29 PM	End	Execution	RFPA - 5977A SQ - Source: EI - Extractor	Run Count : 1
June 25, 2025 3:10:35 PM	start	Execution	Signal to Noise EI - Liquid Injection, Front SSL, SQ - Source: EI - Extractor using Filament 1 - L: >= 1200	None
June 25, 2025 3:10:40 PM	start	Execution	Tune EI - 5977A SQ - Source: EI - Extractor Filament 1 (Qualitative - No setpoints associated)	None
June 25, 2025 4:10:20 PM	start	Execution	Signal to Noise EI - Liquid Injection, Front SSL, SQ - Source: EI - Extractor using Filament 1 - L: >= 1200	None
June 25, 2025 4:10:23 PM	start	Execution	Tune EI - 5977A SQ - Source: EI - Extractor Filament 1 (Qualitative - No setpoints associated)	None
June 25, 2025 4:10:43 PM	End	Execution	Tune EI - 5977A SQ - Source: EI - Extractor Filament 1 (Qualitative - No setpoints associated)	Run Count : 1
June 25, 2025 4:10:45 PM	start	Execution	Tune EI - 5977A SQ - Source: EI - Extractor Filament 2 (Qualitative - No setpoints associated)	None

User Name: supasak.nimsongtham
Report Generated by Hostname: SCG1115HKC

System Id: BKK_EN0259(GM-7)
Print Date: June 25, 2025 8:40:20 PM

GM-7-2025 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
June 25, 2025 4:11:08 PM	End	Execution	Tune EI - 5977A SQ - Source: EI - Extractor Filament 2 (Qualitative - No setpoints associated)	Run Count : 1
June 25, 2025 4:11:11 PM	start	Execution	Signal to Noise EI - Liquid Injection, Front SSL, SQ - Source: EI - Extractor using Filament 1 - L: >= 1200	None
June 25, 2025 4:30:52 PM	start	Execution	Signal to Noise EI - Liquid Injection, Front SSL, SQ - Source: EI - Extractor using Filament 1 - L: >= 1200	None
June 25, 2025 5:23:59 PM	Audit	Data	Signal to Noise EI - Liquid Injection, Front SSL, SQ - Source: EI - Extractor using Filament 1 - L: >= 1200	Data files Path : C:\Users\nimsongth\Download s\OQ data\OQ data\OQ_SN_F1_001.D
June 25, 2025 5:24:18 PM	Audit	Data	DataManager	DataManager was in a data verification state but the user chose to start over
June 25, 2025 5:26:41 PM	Audit	Data	Signal to Noise EI - Liquid Injection, Front SSL, SQ - Source: EI - Extractor using Filament 1 - L: >= 1200	Data files Path : C:\Users\nimsongth\Download s\OQ data\OQ data\OQ_SN_F1_001.D
June 25, 2025 5:27:29 PM	Audit	Reporting	Reintegration	Reintegration Count: 1 --[Integration Type: Inject ion.Baseline Correction Mode: Advanced Initial Slope Sensitivity: 10 Initial Peak Width: 0.01 Initial Area Reject: 0 Initial Height Reject: 20000 Integration: Off at 0 Integration: On at 4]

User Name: supasak.ninsongtham
Report Generated by Hostname: SCG111SHKC
System Id: BKK_EN0259(GM-7)
Print Date: June 25, 2025 8:40:20 PM

GM-7-2025 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
June 25, 2025 5:29:45 PM	End	Execution	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 1 - L: >= 1200	Run Count : 1
June 25, 2025 5:31:32 PM	Audit	TestUnlocked	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 1 - L: >= 1200	Deviation filed for Run Count : 1
June 25, 2025 5:31:32 PM	start	Execution	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 1 - L: >= 1200	None
June 25, 2025 5:34:18 PM	Audit	Data	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 1 - L: >= 1200	Data files Path : C:\Users\msongth\Download s\OQ data\OQ data\OQ_SN_F1_001.D
June 25, 2025 5:35:03 PM	Audit	Data	DataManager	DataManager was in a data verification state but the user chose to start over
June 25, 2025 5:37:01 PM	Audit	Data	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 1 - L: >= 1200	Data files Path : C:\Users\msongth\Download s\OQ data\OQ data\OQ_SN_F1_001.D
June 25, 2025 5:37:47 PM	Audit	Reporting	Reintegration	Reintegration Count: 1 --- [Integration Type: Injection/Baseline Correction Mode: Advanced;Initial Slope Sensitivity: 10;Initial Peak Width: 0.01;Initial Area Reject: 0;Initial Height Reject: 25000;Integration: OFF at 0;Integration: ON at 4]

Page 7 / 9

Date: June 25, 2025 8:40:18 PM
System ID: BKK_EN0259(GM-7)

Page 13 / 16

User Name: supasak.ninsongtham
Report Generated by Hostname: SCG111SHKC
System Id: BKK_EN0259(GM-7)
Print Date: June 25, 2025 8:40:20 PM

GM-7-2025 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
June 25, 2025 5:40:09 PM	End	Execution	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 1 - L: >= 1200	Run Count : 2
June 25, 2025 5:41:09 PM	start	Execution	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 2 - L: >= 1200	None
June 25, 2025 5:44:37 PM	Audit	Data	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 2 - L: >= 1200	Data files Path : C:\Users\msongth\Download s\OQ data\OQ data\OQ_SN_F2_001.D
June 25, 2025 5:48:28 PM	End	Execution	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 2 - L: >= 1200	Run Count : 1
June 25, 2025 5:49:39 PM	Audit	TestUnlocked	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 2 - L: >= 1200	Deviation filed for Run Count : 1
June 25, 2025 5:49:49 PM	start	Execution	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 2 - L: >= 1200	None
June 25, 2025 5:57:10 PM	Audit	Data	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 2 - L: >= 1200	Data files Path : C:\Users\msongth\Download s\OQ data\OQ data\OQ_SN_F2_001.D
June 25, 2025 5:57:46 PM	Audit	Data	DataManager	DataManager was in a data verification state but the user chose to start over

Page 7 / 9

Date: June 25, 2025 8:40:18 PM
System ID: BKK_EN0259(GM-7)

Page 14 / 16

User Name: supasak.ninsongtham
Report Generated by Hostname: SCG111SHKC
System Id: BKK_EN0259(GM-7)
Print Date: June 25, 2025 8:40:20 PM

GM-7-2025 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
June 25, 2025 5:59:51 PM	Audit	Data	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 2 - L: >= 1200	Data files Path : C:\Users\msongth\Download s\OQ data\OQ data\OQ_SN_F2_001.D
June 25, 2025 6:00:02 PM	Audit	Data	DataManager	DataManager was in a data verification state but the user chose to start over
June 25, 2025 6:02:07 PM	Audit	Data	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 2 - L: >= 1200	Data files Path : C:\Users\msongth\Download s\OQ data\OQ data\OQ_SN_F2_001.D
June 25, 2025 6:02:24 PM	Audit	Data	DataManager	DataManager was in a data verification state but the user chose to start over
June 25, 2025 6:19:36 PM	Audit	Data	DataManager	DataManager was in a data verification state but the user chose to start over
June 25, 2025 6:27:38 PM	Audit	Data	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 2 - L: >= 1200	Data files Path : C:\Users\msongth\Download s\OQ data\OQ data\OQ_SN_F2_002.D
June 25, 2025 6:33:07 PM	End	Execution	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 2 - L: >= 1200	Run Count : 2
June 25, 2025 6:34:17 PM	Audit	TestUnlocked	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 2 - L: >= 1200	Deviation filed for Run Count : 2
June 25, 2025 6:34:17 PM	start	Execution	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 2 - L: >= 1200	None

Page 8 / 9

Date: June 25, 2025 8:40:18 PM
System ID: BKK_EN0259(GM-7)

Page 15 / 16

User Name: supasak.ninsongtham
Report Generated by Hostname: SCG111SHKC
System Id: BKK_EN0259(GM-7)
Print Date: June 25, 2025 8:40:20 PM

GM-7-2025 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
June 25, 2025 6:35:07 PM	Audit	AceClosed	Session	None
June 25, 2025 6:35:57 PM	Audit	AceRestarted	Session	Host Name: SCG111SHKC, Drive Serial Number: C3031778
June 25, 2025 6:35:59 PM	Audit	SessionReloaded	Session	None
June 25, 2025 6:36:12 PM	start	Qualification	Session	OQ
June 25, 2025 6:36:13 PM	start	Execution	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 2 - L: >= 1200	None
June 25, 2025 6:39:41 PM	Audit	Data	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 2 - L: >= 1200	Data files Path : C:\Users\msongth\Download s\OQ data\OQ data\OQ_SN_F2_002.D
June 25, 2025 6:42:57 PM	End	Execution	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 2 - L: >= 1200	Run Count : 3
June 25, 2025 6:43:11 PM	End	Qualification	Session	OQ
June 25, 2025 6:43:11 PM	start	Reporting	Session	None
June 25, 2025 8:04:02 PM	Audit	Reporting	Session	Report Generated : Certificate
June 25, 2025 8:32:04 PM	Audit	Reporting	Session	Report Generated : Report

Page 9 / 9

Date: June 25, 2025 8:40:18 PM
System ID: BKK_EN0259(GM-7)

Page 16 / 16

Certificate of System Qualification

GC-OQ

REVIEW BY
APPROVED BY Tanyatorn M.
NEXT CAL. DATE 9 May 26

System ID:	2025_ALS_GC#11_CN2303A021_OQHW
Organization Name:	ALS Laboratory Group (Thailand) Co., Ltd.
Organization Location:	104 Soi 40 Phatthanakan Rd,Khwang Suan Luang, Khet Suan Luang, Bangkok 10250
Date:	May 9, 2025 11:32:14 AM
EQP Name:	AgilentRecommended
EQP Revision:	GC.02.53
Overall Qualification Status:	Pass

CDS Logon Verification - GC

Logon: Saenguthai Tarak

Overall CDS Logon Verification - GC Test Status

Pass

System Inspection and Basic Safety and Operation

Name: 8890

Setpoint Status: Pass

Overall System Inspection and Basic Safety and Operation Test Status

Pass

Inlet Pressure Decay

Name: 8890
Front SSL

Setpoint Status: Pass
Pressure: 25.0 psi
Pressure Change: -0.1 psi /5 minutes
Agilent Recommended: >= -2.0 and <= 0.5

Date: May 9, 2025 11:32:14 AM
System ID: 2025_ALS_GC#11_CN2303A021_OQ

Page 1 / 25

Overall Inlet Pressure Decay Test Status

Pass

Inlet Pressure Accuracy

Name: 8890
Front SSL

Setpoint Status: Pass

	Setpoint		Actual	
Inlet Pressure:	25,0	psi	24,9	psi
Accuracy:			0,1	psi
Agilent Recommended:			<= 1,2	

Overall Inlet Pressure Accuracy Test Status

Pass

Inlet Pressure Decay

Name: 8890
Back SSL

Setpoint Status: Pass
Pressure: 25,0 psi
Pressure Change: -0,1 psi /5 minutes
Agilent Recommended: >= -2,0 and <= 0,5

Overall Inlet Pressure Decay Test Status

Pass

Inlet Pressure Accuracy

Name: 8890
Back SSL

Date: May 9, 2025 11:32:14 AM
System ID: 2025_ALS_GC#11_CN2303A021_OQ

Page 2 / 25

Setpoint Status: Pass

	Setpoint		Actual	
Inlet Pressure:	25,0	psi	24,8	psi
Accuracy:			0,2	psi
Agilent Recommended:			<= 1,2	

Overall Inlet Pressure Accuracy Test Status

Pass

Detector Flow Accuracy

Name: 8890
Front FID

Setpoint Status: Pass
Flow Type: Fuel
Setpoint: 30,0 mL/min Measured Flow: 30,3 mL/min
Accuracy: 0,3 mL/min
Agilent Recommended: <= 10,0 % setpoint (3,0 ml/min)
Limit is percentage of setpoint or 0,5 ml/minute, whichever is largest.

Setpoint Status: Pass
Flow Type: Oxidizer
Setpoint: 400,0 mL/min Measured Flow: 398 mL/min
Accuracy: 2,0 mL/min
Agilent Recommended: <= 10,0 % setpoint (40,0 ml/min)
Limit is percentage of setpoint or 0,5 ml/minute, whichever is largest.

Setpoint Status: Pass
Flow Type: Makeup
Setpoint: 25,0 mL/min Measured Flow: 25,1 mL/min
Accuracy: 0,1 mL/min
Agilent Recommended: <= 10,0 % setpoint (2,5 ml/min)
Limit is percentage of setpoint or 0,5 ml/minute, whichever is largest.

Date: May 9, 2025 11:32:14 AM
System ID: 2025_ALS_GC#11_CN2303A021_OQ

Page 3 / 25

Overall Detector Flow Accuracy Test Status

Pass

Detector Flow Accuracy

Name: 8890
Back FID

Setpoint Status: Pass
Flow Type: Fuel
Setpoint: 30,0 mL/min Measured Flow: 30,1 mL/min
Accuracy: 0,1 mL/min
Agilent Recommended: <= 10,0 % setpoint (3,0 ml/min)
Limit is percentage of setpoint or 0,5 ml/minute, whichever is largest.

Setpoint Status: Pass
Flow Type: Oxidizer
Setpoint: 400,0 mL/min Measured Flow: 391 mL/min
Accuracy: 9,0 mL/min
Agilent Recommended: <= 10,0 % setpoint (40,0 ml/min)
Limit is percentage of setpoint or 0,5 ml/minute, whichever is largest.

Setpoint Status: Pass
Flow Type: Makeup
Setpoint: 25,0 mL/min Measured Flow: 24,8 mL/min
Accuracy: 0,2 mL/min
Agilent Recommended: <= 10,0 % setpoint (2,5 ml/min)
Limit is percentage of setpoint or 0,5 ml/minute, whichever is largest.

Overall Detector Flow Accuracy Test Status

Pass

GC Oven Temperature Accuracy

Name: 8890

Date: May 9, 2025 11:32:14 AM
System ID: 2025_ALS_GC#11_CN2303A021_OQ

Page 4 / 25

Setpoint Status: Pass
Zone: Oven
Setpoint/Actual
Temperature: 230,0 230,4 °C
Accuracy: 0,4 °C
Agilent Recommended: >= -1,0 % setpoint in K (-5,0 °C)
<= 1,0 % setpoint in K (5,0 °C)

Setpoint Status: Pass
Zone: Oven
Setpoint/Actual
Temperature: 100,0 100,2 °C
Accuracy: 0,2 °C
Agilent Recommended: >= -1,0 % setpoint in K (-3,7 °C)
<= 1,0 % setpoint in K (3,7 °C)

Overall GC Oven Temperature Accuracy Test Status

Pass

GC Oven Temperature Stability

Name: 8890

Setpoint Status: Pass
Setpoint/Average
Temperature: 100,0 100,2 °C
Stability: 0,0 °C
Agilent Recommended: <= 0,5

Overall GC Oven Temperature Stability Test Status

Pass

Scouting Run

Tested Combination1 Front SSL / Front FID
Injection Tower
Name: 7693A

Date: May 9, 2025 11:32:14 AM
System ID: 2025_ALS_GC#11_CN2303A021_OQ

Page 5 / 25

Setpoint Status: Completed

Injection Volume on Column: 1,0 uL

Overall Scouting Run Status

Completed

Noise and Drift

Tested Combination1	Front	SSL	/ Front	FID
Name:	8890			

Setpoint Status: Pass

Base Signal: 5,89 pA

	ASTM Noise		Drift
	pA		pA/h
	0,05		1,11
Agilent Recommended:	<= 0,10	<=	2,50
Status:	Pass		Pass

Overall Noise and Drift Test Status

Pass

Injection Precision

Tested Combination1	Front	SSL	/ Front	FID
Name:	7693A			

Setpoint Status: Pass

Injection Volume on Column: 1,0 uL

Area RSD: 0,06 % Retention Time RSD: 0,19 %

Agilent Recommended: <= 3,00 <= 1,00

Overall Injection Precision Test Status

Pass

Signal to Noise

Tested Combination1	Front	SSL	/ Front	FID
	Injection Tower			
Name:	8890			

Setpoint Status: Pass

Signal to Noise: 994826

Agilent Recommended: >= 300000

Overall Signal to Noise Test Status

Pass

Scouting Run

Tested Combination2	Back	SSL	/ Back	FID
	Injection Tower			
Name:	7693A			

Setpoint Status: Completed

Injection Volume on Column: 1,0 uL

Overall Scouting Run Status

Completed

Noise and Drift

Tested Combination2	Back	SSL	/ Back	FID
Name:	8890			

Setpoint Status: Pass

Base Signal: 17,79 pA

	ASTM Noise		Drift
	pA		pA/h
	0,04		0,07
Agilent Recommended:	<= 0,10	<=	2,50
Status:	Pass		Pass

Overall Noise and Drift Test Status

Pass

Injection Precision

Tested Combination2	Back	SSL	/ Back	FID
Name:	7693A			

Setpoint Status: Pass

Injection Volume on Column: 1,0 uL

Area RSD: 0,52 % Retention Time RSD: 0,23 %

Agilent Recommended: <= 3,00 <= 1,00

Overall Injection Precision Test Status

Pass

Signal to Noise

Tested Combination2	Back	SSL	/ Back	FID
	Injection Tower			
Name:	8890			

Setpoint Status: Pass

Signal to Noise: 837739

Agilent Recommended: >= 300000

Overall Signal to Noise Test Status

Pass

Instrument Details

Purpose

This section describes the as found system configuration.

Details

System

System ID	2025_ALS_GC#11_CN2303A021_OQHW
Manufacturer	Agilent Technologies
Name	8890
Flow Data Input	Manual Data
Temperature Data Input	Manual Data or Other Data Logging

Tested Combination1

Injection Technique	Injection Tower
Sampler Identifier	Sampler 1
Inlet	Front
Detector	Front
LTM Included?	No

Tested Combination2

Injection Technique	Injection Tower
Sampler Identifier	Sampler 2
Inlet	Back
Detector	Back
LTM Included?	No

Sampler 1

Manufacturer	Agilent Technologies
Type	Injection Tower
Name	7693A
Model Number	G4513A
Serial Number	CN23125107
Firmware Revision	A.11.07
Usage	Sample Injection
Location	Front
Syringe Volume (uL)	10

Sampler 2

Manufacturer	Agilent Technologies
Type	Injection Tower
Name	7693A
Model Number	G4513A
Serial Number	CN23125121
Firmware Revision	A.11.07
Usage	Sample Injection
Location	Back
Syringe Volume (uL)	10

Sampler 3

Manufacturer	Agilent Technologies
Type	Tray
Name	7693A
Model Number	G4514A
Serial Number	CN23140S4
Firmware Revision	A.12.03
Vial Heater	Not installed

Mainframe 1

Manufacturer	Agilent Technologies
Name	8890
Model Number	G3540A
Serial Number	CN2303A021
Firmware Revision	3.0.3.21
Oven Type	Standard

Inlet 1

Manufacturer	Agilent Technologies
Name	8890
Type	SSL
Location	Front
Carrier Gas	Helium
Control Type	Electronic Pressure Control (EPC)
Purged Inlet	Yes

Inlet 2

Manufacturer	Agilent Technologies
Name	8890
Type	SSL
Location	Back
Carrier Gas	Helium
Control Type	Electronic Pressure Control (EPC)
Purged Inlet	Yes

Detector 1

Manufacturer	Agilent Technologies
Name	8890
Type	FID
Adapter	Capillary
Control Type	Electronic Pressure Control (EPC)
Location	Front
Makeup Gas	Nitrogen

Detector 2

Manufacturer	Agilent Technologies
Name	8890
Type	FID
Adapter	Capillary
Control Type	Electronic Pressure Control (EPC)
Location	Back
Makeup Gas	Nitrogen

Electronic Signature

Purpose

This signature page was created and published because the ACE sign-off action was executed, which is valid for the entire document, including attachments, The ACE sign-off is an electronic signature that requires two distinct identification components: unique username and personal password, The Agilent representative who has delivered this service understands the meaning and legal status of an electronic signature, As a trained official operator, the Agilent representative has a unique password and logon to access ACE and electronically sign this document, (Other e-signatures can be applied to this document using a Document Content Management or other suitable method defined in your data access and control procedures.)

Details

Full Name of Signer:	Saengutthai Tarak
Logged On User Name:	saengutthai_tarak@non_agilent.com
Signature Creation Date:	May 9, 2025
Reason for Signature:	Executed protocol and published this original version of document

ACE Self Qualification Status

The installed version of ACE used to deliver this service passed qualification; the results conform with expected values. The self qualification summary report is available in the session folder location SDS\ClearStore\AceSelfQualification.

Regulatory Disclaimer

This document provides a protocol to verify and record instrument configuration and evidence of proper operation. It has been prepared from our interpretation of applicable regulations as well as industry best practices. The document is designed to provide an important component of a complete compliance package. Validation depends upon many factors and use of this protocol alone does not assure compliance. Agilent Technologies makes no promises or representations as to its sufficiency for any specific regulatory program.

Warranty

Agilent Technologies makes no warranty of any kind to this material, including but not limited to, the implied warranties or merchantability and fitness for a particular purpose, Agilent Technologies shall not be liable for errors contained herein or for incidental or consequential damages in connection with the furnishing, performance, or use of this material.

User Name: saengutthai.tarak System Id: 2025_ALS_GC#11_CN2303A021_OQHW
Report Generated by Hostname: LAPTOP-CQ3SKOMV Print Date: May 9, 2025 11:32:16 AM

2025_ALS_GC11_CN2303A021_OQHW Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
May 8, 2025 1:49:44 PM	Audit	SessionCreated	Session	Host Name: LAPTOP-CQ3SKOMV; Drive Serial Number: 64A9D8A8
May 8, 2025 1:49:44 PM	start	Configuration	Session	None
May 8, 2025 1:49:44 PM	Audit	Entitlement	Licensing	User is Nonpaying and does not require an unlock code
May 8, 2025 1:56:00 PM	Audit	EqpLoaded	Session	EQP details for primary technique [Gc] = File path : [ProtocolPacks/Gc/Configurations/02,53/Gc,02,53.acq], EQP File Name: [Gc,02,53.acq], EQP Name: [AgilentRecommended],Protocol Revision: [Gc,02,53]
May 8, 2025 1:56:02 PM	End	Configuration	Session	None
May 8, 2025 1:56:05 PM	start	Qualification	Session	PM
May 8, 2025 1:56:10 PM	start	Qualification	Session	OQ
May 8, 2025 1:56:10 PM	start	Execution	System Inspection – 8890; - Mainframe	None
May 8, 2025 1:56:45 PM	End	Execution	System Inspection – 8890; - Mainframe	Run Count : 1
May 8, 2025 1:56:47 PM	start	Execution	Mainframe Maintenance – 8890; - Mainframe: 8890	None
May 8, 2025 1:56:56 PM	End	Execution	Mainframe Maintenance – 8890; - Mainframe: 8890	Run Count : 1
May 8, 2025 1:56:58 PM	start	Execution	Inlet Maintenance – Front SSL; - Inlet: 8890	None
May 8, 2025 1:57:57 PM	End	Execution	Inlet Maintenance – Front SSL; - Inlet: 8890	Run Count : 1

User Name: saengutthai.tarak System Id: 2025_ALS_GC#11_CN2303A021_OQHW
Report Generated by Hostname: LAPTOP-CQ3SKOMV Print Date: May 9, 2025 11:32:16 AM

2025_ALS_GC11_CN2303A021_OQHW Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
May 8, 2025 1:58:00 PM	start	Execution	Inlet Maintenance – Back SSL; - Inlet: 8890	None
May 8, 2025 1:58:52 PM	End	Execution	Inlet Maintenance – Back SSL; - Inlet: 8890	Run Count : 1
May 8, 2025 1:58:54 PM	start	Execution	Detector Maintenance – Front FID; - GC Detector: 8890	None
May 8, 2025 1:59:48 PM	End	Execution	Detector Maintenance – Front FID; - GC Detector: 8890	Run Count : 1
May 8, 2025 1:59:50 PM	start	Execution	Detector Maintenance – Back FID; - GC Detector: 8890	None
May 8, 2025 2:00:25 PM	End	Execution	Detector Maintenance – Back FID; - GC Detector: 8890	Run Count : 1
May 8, 2025 2:00:27 PM	start	Execution	Sampler Maintenance – Front Injection Tower; - Sampler: 7693A	None
May 8, 2025 2:00:34 PM	End	Execution	Sampler Maintenance – Front Injection Tower; - Sampler: 7693A	Run Count : 1
May 8, 2025 2:00:56 PM	start	Execution	Sampler Maintenance – Back Injection Tower; - Sampler: 7693A	None
May 8, 2025 2:01:05 PM	End	Execution	Sampler Maintenance – Back Injection Tower; - Sampler: 7693A	Run Count : 1
May 8, 2025 2:01:09 PM	start	Execution	Service Review – 8890; - Qualitative Test – No setpoints associated	None
May 8, 2025 2:01:41 PM	End	Execution	Service Review – 8890; - Qualitative Test – No setpoints associated	Run Count : 1
May 8, 2025 2:01:43 PM	End	Qualification	Session	PM

User Name: seenguthai.tarek System Id: 2025_ALS_GC#11_CN2303A021_OQHW
Report Generated by Hostname: LAPTOP-CQ3SKOMV Print Date: May 9, 2025 11:32:16 AM

2025_ALS_GC11_CN2303A021_OQHW Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
May 8, 2025 2:01:43 PM	start	Qualification	Session	OQ
May 8, 2025 2:01:43 PM	start	Execution	CDS Logon Verification = GC = 8890: = Qualitative test	None
May 8, 2025 2:06:13 PM	End	Execution	CDS Logon Verification = GC = 8890: = Qualitative test	Run Count : 1
May 8, 2025 2:06:16 PM	start	Execution	System Inspection and Basic Safety and Operation = 8890 = Qualitative Test = No setpoints associated	None
May 8, 2025 2:06:30 PM	End	Execution	System Inspection and Basic Safety and Operation = 8890 = Qualitative Test = No setpoints associated	Run Count : 1
May 8, 2025 2:06:43 PM	start	Execution	Inlet Pressure Decay = Front SSL = Pressure Controlled Inlet = S: 25,0 psi = L: >= -2,0 psi and <= 0,5 psi	None
May 8, 2025 2:11:09 PM	End	Execution	Inlet Pressure Decay = Front SSL = Pressure Controlled Inlet = S: 25,0 psi = L: >= -2,0 psi and <= 0,5 psi	Run Count : 1
May 8, 2025 2:11:11 PM	start	Execution	Inlet Pressure Accuracy = Front SSL = Pressure Controlled Inlet = S: 25,0 psi = L: <= 1,2 psi	None
May 8, 2025 2:12:26 PM	End	Execution	Inlet Pressure Accuracy = Front SSL = Pressure Controlled Inlet = S: 25,0 psi = L: <= 1,2 psi	Run Count : 1
May 8, 2025 2:12:27 PM	start	Execution	Inlet Pressure Decay = Back SSL = Pressure Controlled Inlet = S: 25,0 psi = L: >= -2,0 psi and <= 0,5 psi	None

User Name: seenguthai.tarek System Id: 2025_ALS_GC#11_CN2303A021_OQHW
Report Generated by Hostname: LAPTOP-CQ3SKOMV Print Date: May 9, 2025 11:32:16 AM

2025_ALS_GC11_CN2303A021_OQHW Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
May 8, 2025 2:17:04 PM	End	Execution	Inlet Pressure Decay = Back SSL = Pressure Controlled Inlet = S: 25,0 psi = L: >= -2,0 psi and <= 0,5 psi	Run Count : 1
May 8, 2025 2:17:06 PM	start	Execution	Inlet Pressure Accuracy = Back SSL = Pressure Controlled Inlet = S: 25,0 psi = L: <= 1,2 psi	None
May 8, 2025 2:18:01 PM	End	Execution	Inlet Pressure Accuracy = Back SSL = Pressure Controlled Inlet = S: 25,0 psi = L: <= 1,2 psi	Run Count : 1
May 8, 2025 2:18:04 PM	start	Execution	Detector Flow Accuracy = Front FID: = Type : Fuel - S: 30,0 mL/min = L: <= 10,0% setpoint	None
May 8, 2025 2:18:27 PM	Audit	Data	Detector Flow Accuracy = Front FID: = Type : Fuel - S: 30,0 mL/min = L: <= 10,0% setpoint	Manual Data Entry
May 8, 2025 2:18:30 PM	End	Execution	Detector Flow Accuracy = Front FID: = Type : Fuel - S: 30,0 mL/min = L: <= 10,0% setpoint	Run Count : 1
May 8, 2025 2:18:32 PM	start	Execution	Detector Flow Accuracy = Front FID: = Type : Oxidizer = S: 400,0 mL/min = L: <= 10,0% setpoint	None
May 8, 2025 2:19:04 PM	Audit	Data	Detector Flow Accuracy = Front FID: = Type : Oxidizer = S: 400,0 mL/min = L: <= 10,0% setpoint	Manual Data Entry
May 8, 2025 2:19:06 PM	End	Execution	Detector Flow Accuracy = Front FID: = Type : Oxidizer = S: 400,0 mL/min = L: <= 10,0% setpoint	Run Count : 1
May 8, 2025 2:19:08 PM	start	Execution	Detector Flow Accuracy = Front FID: = Type : Makeup = S: 25,0 mL/min = L: <= 10,0% setpoint	None

User Name: seenguthai.tarek System Id: 2025_ALS_GC#11_CN2303A021_OQHW
Report Generated by Hostname: LAPTOP-CQ3SKOMV Print Date: May 9, 2025 11:32:16 AM

2025_ALS_GC11_CN2303A021_OQHW Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
May 8, 2025 2:20:02 PM	Audit	Data	Detector Flow Accuracy = Front FID: = Type : Makeup = S: 25,0 mL/min = L: <= 10,0% setpoint	Manual Data Entry
May 8, 2025 2:20:06 PM	End	Execution	Detector Flow Accuracy = Front FID: = Type : Makeup = S: 25,0 mL/min = L: <= 10,0% setpoint	Run Count : 1
May 8, 2025 2:20:08 PM	start	Execution	Detector Flow Accuracy = Back FID: = Type : Fuel - S: 30,0 mL/min = L: <= 10,0% setpoint	None
May 8, 2025 2:21:13 PM	Audit	Data	Detector Flow Accuracy = Back FID: = Type : Fuel - S: 30,0 mL/min = L: <= 10,0% setpoint	Manual Data Entry
May 8, 2025 2:21:14 PM	End	Execution	Detector Flow Accuracy = Back FID: = Type : Fuel - S: 30,0 mL/min = L: <= 10,0% setpoint	Run Count : 1
May 8, 2025 2:21:17 PM	start	Execution	Detector Flow Accuracy = Back FID: = Type : Oxidizer = S: 400,0 mL/min = L: <= 10,0% setpoint	None
May 8, 2025 2:21:31 PM	Audit	Data	Detector Flow Accuracy = Back FID: = Type : Oxidizer = S: 400,0 mL/min = L: <= 10,0% setpoint	Manual Data Entry
May 8, 2025 2:21:35 PM	End	Execution	Detector Flow Accuracy = Back FID: = Type : Oxidizer = S: 400,0 mL/min = L: <= 10,0% setpoint	Run Count : 1
May 8, 2025 2:21:37 PM	start	Execution	Detector Flow Accuracy = Back FID: = Type : Makeup = S: 25,0 mL/min = L: <= 10,0% setpoint	None
May 8, 2025 2:22:03 PM	Audit	Data	Detector Flow Accuracy = Back FID: = Type : Makeup = S: 25,0 mL/min = L: <= 10,0% setpoint	Manual Data Entry
May 8, 2025 2:22:05 PM	End	Execution	Detector Flow Accuracy = Back FID: = Type : Makeup = S: 25,0 mL/min = L: <= 10,0% setpoint	Run Count : 1

User Name: seenguthai.tarek System Id: 2025_ALS_GC#11_CN2303A021_OQHW
Report Generated by Hostname: LAPTOP-CQ3SKOMV Print Date: May 9, 2025 11:32:16 AM

2025_ALS_GC11_CN2303A021_OQHW Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
May 8, 2025 2:22:08 PM	start	Execution	GC Oven Temperature Accuracy = 8890 = Temperature : Oven = S: 230,0°C = L: >= -1,0 AND <= 1,0 % setpoint in K	None
May 8, 2025 2:23:02 PM	Audit	Data	GC Oven Temperature Accuracy = 8890 = Temperature : Oven = S: 230,0°C = L: >= -1,0 AND <= 1,0 % setpoint in K	Manual Data Entry
May 8, 2025 2:23:07 PM	End	Execution	GC Oven Temperature Accuracy = 8890 = Temperature : Oven = S: 230,0°C = L: >= -1,0 AND <= 1,0 % setpoint in K	Run Count : 1
May 8, 2025 2:23:09 PM	start	Execution	GC Oven Temperature Accuracy = 8890 = Temperature : Oven = S: 100,0°C = L: >= -1,0 AND <= 1,0 % setpoint in K	None
May 8, 2025 2:25:03 PM	Audit	Data	GC Oven Temperature Accuracy = 8890 = Temperature : Oven = S: 100,0°C = L: >= -1,0 AND <= 1,0 % setpoint in K	Manual Data Entry
May 8, 2025 2:25:05 PM	End	Execution	GC Oven Temperature Accuracy = 8890 = Temperature : Oven = S: 100,0°C = L: >= -1,0 AND <= 1,0 % setpoint in K	Run Count : 1
May 8, 2025 2:25:07 PM	start	Execution	GC Oven Temperature Stability = 8890 = Temperature : Oven = S: 100,0°C = L: <= 0,5°C	None
May 8, 2025 2:31:03 PM	Audit	Data	GC Oven Temperature Stability = 8890 = Temperature : Oven = S: 100,0°C = L: <= 0,5°C	Manual Data Entry
May 8, 2025 2:31:04 PM	End	Execution	GC Oven Temperature Stability = 8890 = Temperature : Oven = S: 100,0°C = L: <= 0,5°C	Run Count : 1

User Name: seenguthai.tarek System Id: 2025_ALS_GC#11_CN2303A021_OQHW
Report Generated by Hostname: LAPTOP-CQ3SKOMV Print Date: May 9, 2025 11:32:16 AM

2025_ALS_GC11_CN2303A021_OQHW Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
May 8, 2025 2:31:12 PM	start	Execution	GC Scouting Run - Injection Tower, Front SSL, Front FID: = Part of System Preparation = No limits associated	None
May 8, 2025 2:31:35 PM	Audit	AceClosed	Session	None
May 9, 2025 9:52:28 AM	Audit	AceRestarted	Session	Host Name: LAPTOP-CQ3SKOMV, Drive Serial Number: 64A92D8A8
May 9, 2025 8:32:30 AM	Audit	SessionReloaded	Session	None
May 9, 2025 8:32:46 AM	start	Qualification	Session	PM
May 9, 2025 8:32:46 AM	start	Qualification	Session	OQ
May 9, 2025 8:32:46 AM	start	Execution	GC Scouting Run - Injection Tower, Front SSL, Front FID: = Part of System Preparation = No limits associated	None
May 9, 2025 8:34:41 AM	Audit	Data	GC Scouting Run - Injection Tower, Front SSL, Front FID: = Part of System Preparation = No limits associated	Data files Path : F:\OQ2025\Data\OQGC=1\FrontBOQ_Front_ECF.dx
May 9, 2025 8:34:55 AM	Audit	Reporting	Reintegration	Reintegration Count: 1 – [Integration Type: Injection;Baseline Correction Mode: Advanced;Initial Slope Sensitivity: 10;Initial Peak Width: 0,01;Initial Area Reject: 0;Initial Height Reject: 100;Integration: Off at 0;Integration: On at 0,015;Integration: Off at 0,5]
May 9, 2025 8:35:11 AM	End	Execution	GC Scouting Run - Injection Tower, Front SSL, Front FID: = Part of System Preparation = No limits associated	Run Count : 1

User Name: seenguthai.tarek System Id: 2025_ALS_GC#11_CN2303A021_OQHW
Report Generated by Hostname: LAPTOP-CQ3SKOMV Print Date: May 9, 2025 11:32:16 AM

2025_ALS_GC11_CN2303A021_OQHW Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
May 8, 2025 8:56:15 AM	start	Execution	Noise and Drift = Front FID: = Detector FID = L (Noise): <= 0,10 pA = L (Drift): <= 2,50 pA/hour	None
May 8, 2025 8:56:18 AM	Audit	Data	Noise and Drift = Front FID: = Detector FID = L (Noise): <= 0,10 pA = L (Drift): <= 2,50 pA/hour	Data files Path : F:\OQ2025\Data\OQGC=11_2_nd\BOQ_Front_ND4F.dx
May 9, 2025 8:56:27 AM	End	Execution	Noise and Drift = Front FID: = Detector FID = L (Noise): <= 0,10 pA = L (Drift): <= 2,50 pA/hour	Run Count : 1
May 9, 2025 8:56:31 AM	start	Execution	Injection Precision - Injection Tower, Front SSL, Front FID: = GC = L (Area): <= 3,00% = L (Ret, Time): <= 1,00%	None
May 9, 2025 9:34:24 AM	Audit	Data	Injection Precision - Injection Tower, Front SSL, Front FID: = GC = L (Area): <= 3,00% = L (Ret, Time): <= 1,00%	Data files Path : F:\OQ2025\Data\OQGC=11_Front_IP_nd\BOQ_Front_IP=005.dx
May 9, 2025 9:34:24 AM	Audit	Data	Injection Precision - Injection Tower, Front SSL, Front FID: = GC = L (Area): <= 3,00% = L (Ret, Time): <= 1,00%	Data files Path : F:\OQ2025\Data\OQGC=11_Front_IP_nd\BOQ_Front_IP=006.dx
May 9, 2025 9:34:24 AM	Audit	Data	Injection Precision - Injection Tower, Front SSL, Front FID: = GC = L (Area): <= 3,00% = L (Ret, Time): <= 1,00%	Data files Path : F:\OQ2025\Data\OQGC=11_Front_IP_nd\BOQ_Front_IP=007.dx
May 9, 2025 9:34:24 AM	Audit	Data	Injection Precision - Injection Tower, Front SSL, Front FID: = GC = L (Area): <= 3,00% = L (Ret, Time): <= 1,00%	Data files Path : F:\OQ2025\Data\OQGC=11_Front_IP_nd\BOQ_Front_IP=008.dx

User Name: seenguthai.tarek System Id: 2025_ALS_GC#11_CN2303A021_OQHW
Report Generated by Hostname: LAPTOP-CQ3SKOMV Print Date: May 9, 2025 11:32:16 AM

2025_ALS_GC11_CN2303A021_OQHW Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
May 9, 2025 9:34:24 AM	Audit	Data	Injection Precision - Injection Tower, Front SSL, Front FID: = GC = L (Area): <= 3,00% = L (Ret, Time): <= 1,00%	Data files Path : F:\OQ2025\Data\OQGC=11_Front_IP_nd\BOQ_Front_IP=009.dx
May 9, 2025 9:34:34 AM	Audit	Reporting	Reintegration	Reintegration Count: 1 – [Integration Type: Injection;Baseline Correction Mode: Advanced;Initial Slope Sensitivity: 10;Initial Peak Width: 0,01;Initial Area Reject: 0;Initial Height Reject: 100;Integration: Off at 0;Integration: On at 0,015;Integration: Off at 0,5]
May 9, 2025 9:34:43 AM	End	Execution	Injection Precision - Injection Tower, Front SSL, Front FID: = GC = L (Area): <= 3,00% = L (Ret, Time): <= 1,00%	Run Count : 1
May 9, 2025 9:34:49 AM	start	Execution	Signal to Noise - Injection Tower, Front SSL, Front FID: = Detector FID = L: >= 300000	None
May 9, 2025 9:35:19 AM	Audit	Data	Signal to Noise - Injection Tower, Front SSL, Front FID: = Detector FID = L: >= 300000	Data files Path : F:\OQ2025\Data\OQGC=11_Front_SN_nd\BOQ_Front_SN.dx

User Name: seenguthai.tarek System Id: 2025_ALS_GC#11_CN2303A021_OQHW
Report Generated by Hostname: LAPTOP-CQ3SKOMV Print Date: May 9, 2025 11:32:16 AM

2025_ALS_GC11_CN2303A021_OQHW Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
May 9, 2025 9:35:27 AM	Audit	Reporting	Reintegration	Reintegration Count: 1 – [Integration Type: Injection;Baseline Correction Mode: Advanced;Initial Slope Sensitivity: 10;Initial Peak Width: 0,01;Initial Area Reject: 0;Initial Height Reject: 100;Integration: Off at 0;Integration: On at 0,015;Integration: Off at 0,5]
May 9, 2025 9:35:34 AM	End	Execution	Signal to Noise - Injection Tower, Front SSL, Front FID: = Detector FID = L: >= 300000	Run Count : 1
May 9, 2025 9:35:38 AM	start	Execution	GC Scouting Run - Injection Tower, Back SSL, Back FID: = Part of System Preparation = No limits associated	None
May 9, 2025 9:46:40 AM	Audit	Data	GC Scouting Run - Injection Tower, Back SSL, Back FID: = Part of System Preparation = No limits associated	Data files Path : F:\OQ2025\Data\BackOQGC=11_Back_IP=1_nd\BOQ_Back_SC.dx
May 9, 2025 9:46:57 AM	End	Execution	GC Scouting Run - Injection Tower, Back SSL, Back FID: = Part of System Preparation = No limits associated	Run Count : 1
May 9, 2025 9:47:00 AM	start	Execution	Noise and Drift - Back FID: = Detector FID = L (Noise): <= 0,10 pA = L (Drift): <= 2,50 pA/hour	None
May 9, 2025 10:51:06 AM	Audit	Data	Noise and Drift - Back FID: = Detector FID = L (Noise): <= 0,10 pA = L (Drift): <= 2,50 pA/hour	Data files Path : F:\OQ2025\Data\BackOQGC=11_Back_ND-2_nd\BOQ_Back_ND4F.dx

User Name: seenguthai.tarek System Id: 2025_ALS_GC#11_CN2303A021_OQHW
Report Generated by Hostname: LAPTOP-CQ3SKOMV Print Date: May 9, 2025 11:32:16 AM

2025_ALS_GC11_CN2303A021_OQHW Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
May 9, 2025 10:51:12 AM	End	Execution	Noise and Drift = Back FID: = Detector FID = L (Noise): <= 0,10 pA = L (Drift): <= 2,50 pA/hour	Run Count : 1
May 9, 2025 10:51:16 AM	start	Execution	Injection Precision - Injection Tower, Back SSL, Back FID: = GC = L (Area): <= 3,00% = L (Ret, Time): <= 1,00%	None
May 9, 2025 11:09:34 AM	Audit	Data	Injection Precision - Injection Tower, Back SSL, Back FID: = GC = L (Area): <= 3,00% = L (Ret, Time): <= 1,00%	Data files Path : F:\OQ2025\Data\BackOQGC=11_Back_IP=1_nd\BOQ_Back_IP=001.dx
May 9, 2025 11:09:34 AM	Audit	Data	Injection Precision - Injection Tower, Back SSL, Back FID: = GC = L (Area): <= 3,00% = L (Ret, Time): <= 1,00%	Data files Path : F:\OQ2025\Data\BackOQGC=11_Back_IP=1_nd\BOQ_Back_IP=002.dx
May 9, 2025 11:09:34 AM	Audit	Data	Injection Precision - Injection Tower, Back SSL, Back FID: = GC = L (Area): <= 3,00% = L (Ret, Time): <= 1,00%	Data files Path : F:\OQ2025\Data\BackOQGC=11_Back_IP=1_nd\BOQ_Back_IP=003.dx
May 9, 2025 11:09:34 AM	Audit	Data	Injection Precision - Injection Tower, Back SSL, Back FID: = GC = L (Area): <= 3,00% = L (Ret, Time): <= 1,00%	Data files Path : F:\OQ2025\Data\BackOQGC=11_Back_IP=1_nd\BOQ_Back_IP=004.dx
May 9, 2025 11:09:34 AM	Audit	Data	Injection Precision - Injection Tower, Back SSL, Back FID: = GC = L (Area): <= 3,00% = L (Ret, Time): <= 1,00%	Data files Path : F:\OQ2025\Data\BackOQGC=11_Back_IP=1_nd\BOQ_Back_IP=005.dx
May 9, 2025 11:09:34 AM	Audit	Data	Injection Precision - Injection Tower, Back SSL, Back FID: = GC = L (Area): <= 3,00% = L (Ret, Time): <= 1,00%	Data files Path : F:\OQ2025\Data\BackOQGC=11_Back_IP=1_nd\BOQ_Back_IP=006.dx

© 2025 by Agilent Technologies

User Name: saengutha\.tarak
Report Generated by Hostname: LAPTOP-CQ3SKOMV

System Id: 2025_ALS_GC#11_CN2303A021_OQHW
Print Date: May 9, 2025 11:32:16 AM

2025_ALS_GC11_CN2303A021_OQHW Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
May 9, 2025 11:09:46 AM	End	Execution	Injection Precision - Injection Tower, Back SSL, Back FID - GC ~L (Area): <= 3,00% ~L (Ret. Time): <= 1,00%	Run Count : 1
May 9, 2025 11:09:49 AM	start	Execution	Signal to Noise - Injection Tower, Back SSL, Back FID - Detector FID ~L: >= 300000	None
May 9, 2025 11:16:51 AM	Audit	Data	Signal to Noise - Injection Tower, Back SSL, Back FID - Detector FID ~L: >= 300000	Data files Path : F:\OQ\2025\Data\Back\OQGC ~11_Back_SN,nBTOQ_Back_SC.dx
May 9, 2025 11:17:07 AM	End	Execution	Signal to Noise - Injection Tower, Back SSL, Back FID - Detector FID ~L: >= 300000	Run Count : 1
May 9, 2025 11:17:11 AM	End	Qualification	Session	OQ
May 9, 2025 11:17:11 AM	start	Reporting	Session	None
May 9, 2025 11:24:47 AM	Audit	Reporting	Session	Report Generated : Report
May 9, 2025 11:25:23 AM	Audit	Reporting	Session	Report Signed : Report PDF Name: 2025_ALS_GC11_CN2303A 021_OQHW_20250509_PM Report_1.pdf User Name: saengutha\.tarak@ron.agilen t.com Full Name of Signer: Saengutha\ Tarak Reason for signature: Executed protocol and published this original version of document
May 9, 2025 11:30:23 AM	Audit	Reporting	Session	Report Generated : Certificate

© 2025 by Agilent Technologies

Agilent CrossLab Compliance Services

User Name: saengutha\.tarak
Report Generated by Hostname: LAPTOP-CQ3SKOMV

System Id: 2025_ALS_GC#11_CN2303A021_OQHW
Print Date: May 9, 2025 11:32:16 AM

2025_ALS_GC11_CN2303A021_OQHW Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
May 9, 2025 11:31:17 AM	Audit	Reporting	Session	Report Generated : Report

Date: May 9, 2025 11:32:14 AM
System ID: 2025_ALS_GC#11_CN2303A021_OQ

Date: May 9, 2025 11:32:14 AM
System ID: 2025_ALS_GC#11_CN2303A021_OQ

TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL.0-2717-3000-29 FAX.0-2719-9484

ilac-MRA
NSC-TH0-TH017025
CALIBRATION 0008

Certificate of Calibration

Cert.No.: 25CH709/1
Page.: 1 of 3

This Certificate was issued to re place to the Certificate No.25CH709

Equipment :	pH Meter
Manufacturer :	Mettler Toledo
Model :	SevenExcellence
Serial No. :	B834291445
ID No. :	RYG_EN0152
Condition As-Received:	Used Item
Received Date :	12 June 2025
Calibration Date :	18 June 2025
Reference :	2506-0407DSC-2
Submitted by :	***ALS Laboratory Group (Thailand) Co.,Ltd. Rayong Branch 616/10 Moo 5, T.Maenam Khu, A.Pluakdaeng, Rayong 21140, Thailand***
Ambient Temperature :	(25 ± 2.5) °C
Relative Humidity :	(50 ± 15) %
Calibration Procedure :	In - house method : - CP-CH5 by direct measurement with DC voltage standard and direct measurement with certified reference material (CRM) - CP-CH8 by comparison with temperature standard

REVIEW BY ..... PhatchanaS
APPROVED BY .....
NEXT CAL DATE..... 18/12/26

Calibrated by : Walalak Sirithean
Approved by : Saithip
Approved Signatory

( ) Chakrit Waewwanjua
( ) Ponpan Palpim
(✓) Saithip Meangmai

Issue Date : 1 July 2025

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

Condition of this calibration result

1. Reference Standard Instrument

Instrument	Serial No.	ID No.	Cert. No.	Due Date
1) Document Process Calibrator	54033049	130RC116	24E2759	25 Aug 2025
2) Ref. Standard Thermometer	498z054	110RC044	24I757	14 July 2025

- This measurement result is traceable to SI throught Technology Promotion Association (Thailand - Japan)

2. Certified Reference Materials :The measurement results are traceable to SI through Hach Lenge GmbH Ltd., Deutsche Akkreditierungsstelle, Accredited No.D-RM-15184-01-00 :The measurement results are traceable to SI through CPA chem Ltd., ANSI-ASQ National Accreditation Board, Accredited No. AR-1835

Buffer Solution	Manufacturer	Lot No.	Exp. date
pH 4.007	CPA chem	1066665	18 Jan 2027
pH 7.000	Hach Lenge GmbH	C03232	02 Dec 2026
pH 10.010	CPA chem	1066669	18 Jan 2026

3. This certificate is valid only to the item calibrated on date and place of calibration.

Calibration Results

Function : mV Measurement

Performing standard curve by Document Process Calibrator at pH (4,7,10)

Unit Under Calibration	Nominal Value	Standard Voltage Input	Actual Reading		Uncertainty of Measurement	Coverage factor
	pH	mV	mV	pH	(±mV)	*k*
pH Meter	4.000	177.48	177.3	4.000	0.058	2.00
S/N.: B834291445	7.000	0.00	-0.1	7.000	0.058	2.00
	10.000	-177.48	-177.5	10.000	0.058	2.00

Calibration Results

Function : pH Measurement

Performing three buffers standard curve by using buffer nominal pH (4,7,10)

Unit Under Calibration	Standard pH Buffer Solution	Actual pH Reading	Actual mV Reading (mV)	Uncertainty of pH Measurement (±)	Coverage factor *k*
pH Electrode	4.007	4.006	181.1	0.0044	2.00
S/N.: 5211504	7.000	7.000	4.9	0.0084	2.00
	10.010	10.007	-170.6	0.0066	2.00

Function : Temperature Measurement

(*) Without adjustment

This equipment was connected with Temperature Probe;
- Model : InLabExpert Pro-ISM
- Serial No. : 5211504
Dimension of probe
- Length : 120 mm.
- Diameter : 12 mm.
- Immersion Depth : 100 mm.

Calibration Point (°C)	Standard Temperature (°C)	UUC* Reading (°C)	Error (°C)	Uncertainty of measurement (± °C)	Coverage factor *k*
25.0	25.001	25.1	0.099	0.13	2.00

Remark - UUC* = Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG, BANGKOK 10250
TEL. 0-2717-3000-24 FAX. 0-2719-9484

ilac-MRA
NSC-TH0-TH017025
CALIBRATION 0008

Certificate of Calibration

Certificate No. : 25E1979/1
Page : 1 of 2

This Certificate was issued to replace to the Certificate No. 25E1979

Equipment :	pH Meter
Manufacturer:	Mettler Toledo
Model :	SevenExcellence
Serial No.:	B834291445
ID No.:	RYG_EN0152
Condition As-Received:	Used Item
Received Date:	12 June 2025
Calibration Date:	16 June 2025
Reference:	2506-0407DSC
Ambient Temperature:	(23 ± 2) °C
Relative Humidity:	(50 ± 10) %
Submitted by:	***ALS Laboratory Group (Thailand) Co.,Ltd. Rayong Branch 616/10 Moo 5, T.Maenam Khu, A.Pluakdaeng, Rayong 21140, Thailand***

This certificate may not be reproduced other than in full, except with the prior written approval of the head of Corporate Services 3: Equipment Calibration and Testing Services.

Procedure used: Calibration were conducted using calibration procedure No. CP-E17 According to EURAMET cg-18.

Condition of this result of calibration

1.Reference standards instruments :

Instrument	Model	Serial No.	Certificate No.	Due Date
1) Multi-Product Calibrator	5500A	8315011	25E1627	19 May 2026

2.This result of calibration was made on requested at the point specified by customer.

3.The certificate is valid only to the item calibrated on date and place of calibration.

4.This measurement result is traceable to the International System of Unit maintained through:-
-Technology Promotion Association (Thailand-Japan), NSC-ONSC Accredited No. Calibration 0008

Calibrated by : Wutchareepom Peethong
Issue Date : 01 July 2025

Approved Signatory :
[ ] Phalinee Prabpaipal
[✓] Nuntawat Khamchai
[ ] Pongsagorn Boonyaporn

Result of calibration :- (*) Without adjustment ( ) After adjustment

Function: DC voltage measurement **Range:** 2000 mV

Standard Value (mV)	UUC* Reading (mV)	Error (mV)	Uncertainty (± µV)
-200.0000	-199.9	0.1	68
-150.0000	-150.0	0.0	65
-100.0000	-100.0	0.0	63
-50.0000	-50.0	0.0	61
0.0000	0.0	0.0	58
50.0000	50.0	0.0	61
100.0000	100.0	0.0	63
150.0000	149.9	-0.1	65
200.0000	199.9	-0.1	68

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k = 2, providing a level of confidence of approximately 95 %

UUC* = Unit Under Calibration.

-o0o-