

ภาคผนวก จ

เอกสารสอบเทียบเครื่องมือที่ใช้ในการตรวจวิเคราะห์

List of Instrument Certificates for Environmental Quality Analysis

No.	Instrument/Equipment	Parameter	Manufacturer	Model/Serial No.	Calibrator	Certification No.	Date of Calibration	Due date of Calibration*
1	Analytical Balance	FAT OIL AND GREASE	Mettler Toledo	AB204-S/FACT / 1129361010	United Analyst and Engineering Consultant Co., Ltd.	250422 1 BL002 25	23/4/2025	22/4/2026
2	Analytical Balance	TOTAL DISSOLVED SOLIDS	Mettler Toledo	XSR205DU / C210685394	National Food Institute,Ministry of Industry, Thailand	25022226-002-01	20/3/2025	19/3/2026
3	Analytical Balance	TOTAL SUSPENDED SOLIDS	Mettler Toledo	XSR205DU / C009071872	National Food Institute,Ministry of Industry, Thailand	25022226-001-01	20/3/2025	19/3/2026
4	BOD Incubator	BIOCHEMICAL OXYGEN DEMAND	ARCO	UR-1320 / -	Technology Promotion Association (Thailand-Japan)	25TM578	19/3/2025	18/3/2026
5	BOD Incubator	BIOCHEMICAL OXYGEN DEMAND	ARCO	UR-1320 / -	Technology Promotion Association (Thailand-Japan)	25TM577	19/3/2025	19/3/2026
6	DO Meter	BIOCHEMICAL OXYGEN DEMAND	YSI	5100 / 11B 101863	Technology Promotion Association (Thailand-Japan)	25TW29	17/2/2025	16/2/2026
7	Hot Air Oven	TOTAL DISSOLVED SOLIDS TOTAL SUSPENDED SOLIDS	Memmert	UF55 / B212.0411	Technology Promotion Association (Thailand-Japan)	25TM579	19/3/2025	18/3/2026
8	Kjeltec Distillation Unit	TOTAL KIELDAHL NITROGEN	FOSS	DT2520 / 91905060	FOSS South East Asia	13852	25/2/2025	24/2/2026
9	Kjeltec System Distilling Unit	TOTAL KIELDAHL NITROGEN	Foss Tecator (Labtec)	KT200 / 91790524	FOSS South East Asia	13319	27/1/2025	26/1/2026
10	Kjeltec Distillation Unit	TOTAL KIELDAHL NITROGEN	FOSS	Kjeltec 8100 / 91889052	FOSS South East Asia	13854	24/2/2025	23/2/2026
11	pH Meter	pH	EcoSense	pH100A / JC04744	Technology promotion association (thailand-japan)	25CH408	3/4/2025	2/4/2026
12	pH Meter	pH	Horiba	LAQUA-PH210 / HA9M0046	technology promotion association (thailand-japan)	24CH1596	26/12/2024	24/12/2025
13	pH Meter	pH	Horiba	LAQUA-PH210 / HA9M0048	technology promotion association (thailand-japan)	25CH586	21/5/2025	19/5/2026
14	pH Meter	pH	Horiba	LAQUA-PH210 / HA0A0005	technology promotion association (thailand-japan)	24CH1597	26/12/2024	24/12/2025
15	pH Meter	pH	Horiba	LAQUA-PH210 / HA9M0047	technology promotion association (thailand-japan)	25CH354	20/3/2025	18/3/2026
16	pH Meter	pH	Horiba	LAQUA-PH210 / HA0C0025	technology promotion association (thailand-japan)	25CH261	26/2/2025	25/3/2026

Certificate of Calibration

Certificate No.: 250422-1-BL002-25

Code No.: BL002-25

Page: 1 of 3

Customer Name: United Analyst and Engineering Consultant Co., Ltd.
Address: 3 Soi Udom suk 41, Sukhumvit Rd., Bang Chak, Phar Khanong, Bangkok 10260

Equipment: Electronic Balance

Manufacturer: Mettler Toledo

Model: AB204-S/FACT

Serial No.: 1129361010

Asset No. : UAE.WAS.002/2552

Building : N/A

Floor : 1

Room : 107

Received Date: April 22, 2025

Date of Calibration : April 23, 2025

Calibration Conditions:	Temperature	22.8 °C	to	23.4 °C
	Humidity	54.8 %	to	68.9 %
	Pressure	756.6 mmHg	to	758.2 mmHg

Calibrated by: Sakkarin Srirahang

Approved by: Suwit Chotnok

Signature:



Issued Date: April 25, 2025

Note : 1) The Uncertainties are for a confidence probability of approximately 95%

2) This Certificate is valid only to the item calibrated on date and place of calibration.

3) This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the United Analyst and Engineering Consultant Co.,Ltd. (UAE)

เอกสารไม่ควบคุม

Certificate No.: 250422-1-BL002-25

Code No.: BL002-25

Page: 2 of 3

Equipment: Electronic Balance

Manufacturer: Mettler Toledo

Model: AB204-S/FACT

Readability: 0.0001 g

Serial No.: 1129361010

ID No.: UAE.WAS.002/2552

Max. Capacity: 220 g

Calibration Date: April 23, 2025

Condition As-Received: In Condition

Condition of Equipment:

Condition of This Result of Calibration:

1. Calibration Method: This instrument was calibrated by method UAE.CP.CAL.006 In-House Method based on UKAS Lab 14 : 2022

2. Reference Standards:

Reference Standard:	Model	Serial No.	Calibrated By	Certificate No.	Traceability	Due Date
Standard Weight Class E2 (OIML)	1 mg to 1 kg	8749109122	AMARC	25-009359	Mettler-Toledo	21-Jan-27
Standard Weight Class F1 (OIML)	1 mg to 200 g	11119512	AMARC	24-013840	Mettler-Toledo	04-Feb-26
Instrument	Model	Serial No.	Calibrated By	Certificate No.	Traceability	Due Date
Thermo-Hygro-Baro Meter	MHB-382SD	AK.46457	SUCCESS	SG-H-00997/67	Success Gateway	21-Nov-25
Thermo-Hygro-Baro Meter	MHB-382SD	AK.46457	TPA	25P795	TPA	25-Feb-26

3. This certification is traceable to SI Unit

4. This certification was certified only for the instrument we calibrated

5. This result of calibration was found accurate as shown on date and place of calibration only.

6. Through the reference standard laboratory of AMARC 25-009359 Calibration 0152

Calibration Result:




1. Repeatability of Reading:

Nominal Value (g)	Standard Deviation of Reading (g)
200*	0.000045

2. Eccentric or off-center loading

A mass of 100 g was placed and moved to various positions on pan

The Balance reading obtained is given in the table.



1 (g)	2 (g)	3 (g)	4 (g)	5 (g)	Maximum Difference (g)
100.0000	99.9996	99.9997	100.0003	100.0005	0.0005

เอกสารไม่ครบถ้วน

Calibration Certificate

Certificate No.: 2502226-002-01
Client name: UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.
Address: 3 Soi Udomsuk 41, Sukhumvit Road,
Bangchack, Prakanong, Bangkok 10260

Page 1 of 4

Equipment: Electronic Balance
Manufacturer: METTLER TOLEDO
Model: XSR205DU
Serial No.: C210685394
ID No.: UAE.WAO.010/2565
Order No.: 2502226
Operation No.: 2502226-002
Date of Receipt: 19 March 2025
Date of Calibration: 20 March 2025

Calibrated by Mr.Yothin Charoensuk
Scientist

Approved by 
(Mr.Pheraphat Tuanjit)

Manager, Division of Calibration Laboratory

Date of Issue: 25 March 2025

Responsible for the Technical Management Team

The uncertainties are for a confidence probability of approximately 95%

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the National Food Institute.

E-CS-009 Revision: 01 Date: 20-04-65



Calibration Report

Certificate No.: 2502226-002-01

Equipment:

Electronic Balance

Manufacturer: METTLER TOLEDO

Model: XSR205DU

Resolution: 0.00001 g / 0.0001 g

Serial No.: C210685394

ID No.: UAE.WAO.010/2565

Capacity: 82 g / 220 g

Date of Calibration: 20 March 2025

Page 2 of 4

Environment Condition: Ambient Temperature: 21.2 ± 0.6 °C Relative Humidity: 48 ± 3.5 %

Place of Calibration: 208 Balance Room, UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.

Condition of Equipment: Good Condition

Condition of This Results of Calibration:

1. Calibration Method: NFI Method W-MA-001 In-House Method based on UKAS Lab 14 : 2019

2. Reference Standards:

Reference Standard	Model	Serial No.	Calibrated By	Certificate No.	Due Date
Standard Weight Class E2	1mg to 200g	B505567572	TCS	M2404100S	19 April 2025
Instrument	Model	Serial No.	Calibrated By	Certificate No.	Due Date
Thermo-Hygro Meter	608-H1	NFI.BTH 017/23	Quality Reborn	QR25-0542	10 February 2026

3. This certification is traceable to SI UNIT

4. This certificate was certified only for the instrument we calibrated.

5. This result of calibration was found accurate as shown on date and place of calibration only.

Calibration Results:




1. Repeatability of Reading:

Nominal Value (g)	Standard Deviation of Reading (g)
40	0.0000042
80	0.0000042
100	0.000000
200	0.000000

2. Off-Center Error:

A mass of 100 g was placed and moved to various position on pan.

The balance reading obtained is given in the table.



1	2	3	4	5	6	(Maximum Difference)
(g)	(g)	(g)	(g)	(g)	(g)	(g)
100.0001	100.0001	100.0001	100.0001	100.0001	100.0001	0.0000

for N. nigredat



Calibration Report

Certificate No.: 2502226-002-01

Equipment:

Electronic Balance

Manufacturer: METTLER TOLEDO

Model: XSR205DU

Resolution: 0.00001 g / 0.0001 g

Serial No.: C210685394

ID No.: UAE.WAO.010/2565

Capacity: 82 g / 220 g

Date of Calibration: 20 March 2025

Page 3 of 4

Calibration Results: (Continued)

Calibration Range: 0-80 g

Calibration Adjustment: Internal Calibration

3. Departure from Nominal Value: (Range: 0 - 82 g ; Resolution: 0.00001 g)

Nominal Value (g)	Standard Value (g)	Average Reading (g)	Correction (g)	Uncertainty (± g)	Coverage Factor k
Unload	0.000000	0.00000	0.00000	0.0000087	2.00
0.001	0.001003	0.00100	0.00000	0.0000090	2.00
0.005	0.005002	0.00501	-0.00001	0.0000092	2.00
0.01	0.010003	0.01002	-0.00002	0.0000089	2.00
0.05	0.049996	0.05001	-0.00001	0.0000096	2.00
0.1	0.100011	0.10002	-0.00001	0.000011	2.00
0.5	0.500016	0.50004	-0.00002	0.000014	2.00
1	1.000003	1.00005	-0.00005	0.000016	2.00
2	2.000023	2.00006	-0.00004	0.000017	2.00
5	5.000015	5.00006	-0.00005	0.000020	2.00
10	10.000009	10.00005	-0.00004	0.000026	2.00
20	20.000030	20.00007	-0.00004	0.000037	2.00
30	30.000039	30.00009	-0.00005	0.000050	2.00
50	50.000028	50.00008	-0.00005	0.000068	2.00
80	80.000067	80.00013	-0.00006	0.00011	2.00



Calibration Report

Certificate No.: 2502226-002-01

Equipment:

Electronic Balance

Manufacturer: METTLER TOLEDO

Model: XSR205DU

Resolution: 0.00001 g / 0.0001 g

Serial No.: C210685394

ID No.: UAE.WAO.010/2565

Capacity: 82 g / 220 g

Date of Calibration: 20 March 2025

Page 4 of 4

Calibration Results: (Continued)

Calibration Range: >80-200 g

Calibration Adjustment: Internal Calibration

3. Departure from Nominal Value: (Range: >80 - 200 g ; Resolution: 0.0001 g)

Nominal Value (g)	Standard Value (g)	Average Reading (g)	Correction (g)	Uncertainty (± g)	Coverage Factor <i>k</i>
90	90.00010	90.0002	-0.0001	0.00015	2.00
100	100.00006	100.0001	0.0000	0.00016	2.00
110	110.00007	110.0002	-0.0001	0.00017	2.00
120	120.00009	120.0002	-0.0001	0.00018	2.00
130	130.00010	130.0002	-0.0001	0.00019	2.00
140	140.00013	140.0002	-0.0001	0.00019	2.00
150	150.00009	150.0002	-0.0001	0.00021	2.00
160	160.00010	160.0002	-0.0001	0.00022	2.00
170	170.00012	170.0002	-0.0001	0.00023	2.00
200	200.00013	200.0002	-0.0001	0.00028	2.00

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k* , providing a level of confidence of approximately 95 %.

----- End -----

for N. ninyabunt

F-CS-012 Revision: 01 Date: 20-04-65



Calibration Certificate

Certificate No.: 2502226-001-01
Client name: UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.
Address: 3 Soi Udomsuk 41, Sukhumvit Road,
Bangchack, Prakhnong, Bangkok 10260

Page 1 of 4

Equipment: Electronic Balance
Manufacturer: METTLER TOLEDO
Model: XSR205DU
Serial No.: C009071872
ID No.: UAE.WAO.012/2563
Order No.: 2502226
Operation No.: 2502226-001
Date of Receipt: 19 March 2025
Date of Calibration: 20 March 2025

Calibrated by Mr.Yothin Charoensuk
Scientist

Approved by 
(Mr.Pheraphat Tuanjit)
Manager, Division of Calibration Laboratory

Date of Issue: 25 March 2025

Responsible for the Technical Management Team

The uncertainties are for a confidence probability of approximately 95%

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the National Food Institute.

F-CS-009 Revision: 01 Date: 20-04-65

Calibration Report

Certificate No.: 2502226-001-01

Equipment:

Electronic Balance

Manufacturer: METTLER TOLEDO

Model: XSR205DU

Resolution: 0.00001 g / 0.0001 g

Serial No.: C009071872

ID No.: UAE.WAO.012/2563

Capacity: 82 g / 220 g

Date of Calibration: 20 March 2025

Page 2 of 4

Environment Condition: Ambient Temperature: 21.2 ± 0.6 °C Relative Humidity: 48 ± 3.5 %

Place of Calibration: 208 Balance Room, UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.

Condition of Equipment: Good Condition

Condition of This Results of Calibration:

1. Calibration Method: NFI Method W-MA-001 In-House Method based on UKAS Lab 14 : 2019

2. Reference Standards:

Reference Standard	Model	Serial No.	Calibrated By	Certificate No.	Due Date
Standard Weight Class E2	1mg to 200g	B505567572	TCS	M2404100S	19 April 2025

Instrument	Model	Serial No.	Calibrated By	Certificate No.	Due Date
Thermo-Hygro Meter	608-H1	NFI.BTH 017/23	Quality Reborn	QR25-0542	10 February 2026

3. This certification is traceable to SI UNIT

4. This certificate was certified only for the instrument we calibrated.

5. This result of calibration was found accurate as shown on date and place of calibration only.

Calibration Results:




1. Repeatability of Reading:

Nominal Value (g)	Standard Deviation of Reading (g)
40	0.0000052
80	0.0000042
100	0.0000000
200	0.0000000

2. Off-Center Error:

A mass of 100 g was placed and moved to various position on pan.

The balance reading obtained is given in the table.



1	2	3	4	5	6	(Maximum Difference)
(g)	(g)	(g)	(g)	(g)	(g)	(g)
100.0001	100.0001	100.0001	100.0001	100.0001	100.0002	0.0001

for N. mignobut

F-CS-012 Revision: 01 Date: 20-04-65

Calibration Report

Certificate No.: 2502226-001-01

Equipment:

Electronic Balance

Manufacturer: METTLER TOLEDO

Model: XSR205DU

Resolution: 0.00001 g / 0.0001 g

Serial No.: C009071872

ID No.: UAE.WAO.012/2563

Capacity: 82 g / 220 g

Date of Calibration: 20 March 2025

Page 3 of 4

Calibration Results: (Continued)

Calibration Range: 0-80 g

Calibration Adjustment: Internal Calibration

3. Departure from Nominal Value: (Range: 0 - 82 g ; Resolution: 0.00001 g)

Nominal Value (g)	Standard Value (g)	Average Reading (g)	Correction (g)	Uncertainty (± g)	Coverage Factor k
Unload	0.000000	0.00000	0.00000	0.0000089	2.00
0.001	0.001003	0.00100	0.00000	0.0000092	2.00
0.005	0.005002	0.00500	0.00000	0.0000094	2.00
0.01	0.010003	0.01000	0.00000	0.0000091	2.00
0.05	0.049996	0.05000	0.00000	0.0000098	2.00
0.1	0.100011	0.10000	0.00001	0.000011	2.00
0.5	0.500016	0.50000	0.00002	0.000014	2.00
1	1.000003	1.00001	-0.00001	0.000016	2.00
2	2.000023	2.00005	-0.00003	0.000017	2.00
5	5.000015	5.00005	-0.00003	0.000021	2.00
10	10.000009	10.00005	-0.00004	0.000026	2.00
20	20.000030	20.00012	-0.00009	0.000037	2.00
30	30.000039	30.00012	-0.00008	0.000050	2.00
50	50.000028	50.00014	-0.00011	0.000068	2.00
80	80.000067	80.00020	-0.00013	0.00011	2.00



for N. Niyasat

Calibration Report

Certificate No.: 2502226-001-01

Equipment:

Electronic Balance

Manufacturer: METTLER TOLEDO

Model: XSR205DU

Resolution: 0.00001 g / 0.0001 g

Serial No.: C009071872

ID No.: UAE.WAO.012/2563

Capacity: 82 g / 220 g

Date of Calibration: 20 March 2025

Page 4 of 4

Calibration Results: (Continued)

Calibration Range: >80-200 g

Calibration Adjustment: Internal Calibration

3. Departure from Nominal Value: (Range: >80 - 200 g ; Resolution: 0.0001 g)

Nominal Value (g)	Standard Value (g)	Average Reading (g)	Correction (g)	Uncertainty (± g)	Coverage Factor <i>k</i>
90	90.00010	90.0002	-0.0001	0.00015	2.00
100	100.00006	100.0001	0.0000	0.00016	2.00
110	110.00007	110.0001	0.0000	0.00017	2.00
120	120.00009	120.0002	-0.0001	0.00018	2.00
130	130.00010	130.0002	-0.0001	0.00019	2.00
140	140.00013	140.0002	-0.0001	0.00019	2.00
150	150.00009	150.0002	-0.0001	0.00021	2.00
160	160.00010	160.0002	-0.0001	0.00022	2.00
170	170.00012	170.0002	-0.0001	0.00023	2.00
200	200.00013	200.0002	-0.0001	0.00028	2.00

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k* , providing a level of confidence of approximately 95 %.

----- End -----

for N. nigudat

E-CS-012 Revision: 01 Date: 20-04-65





TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL.0-2717-3000-29 FAX.0-2719-9484



Certificate of Calibration

Cert. No.: 25TM578

Page : 1 of 3

Equipment : BOD Incubator

Manufacturer : ARCO

Model : UR-1320

Serial No. : -

ID No. : UAE.WAO.006/2553

Submitted by : United Analyst and Engineering Consultant Co.,Ltd.
3 Soi Udomsuk 41, Sukhumvit Road,
Bangchak, Phrakhanong,
Bangkok 10260

Location : Lab Floor 2

Received Order : 19 March 2025

Calibration Date : 19 March 2025

Ambient Temperature : (26 ± 10) °C

Relative Humidity : (50 ± 30) %

AC Line Voltage : (220 ± 22) V

Calibrated by : Man Pattanapongpaiboon

Approved by : 
Approved Signatory

() Chakrit Waewwanjua
() Suwit Imjai
(✓) Kunchit Promprat

Issue Date : 27 March 2025

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

เอกสารไม่ควบคุม



Equipment : BOD Incubator
 Condition As-Received : Used Item
 Reference : 2503-0437OC-2

Cert. No.: 25TM578

Page : 2 of 3

Procedure Used :-

Calibration were conducted using calibration procedure CP-OT02 based on TLAS G-20 according to direct measurement method with Data Acquisition which connected with Resistance Temperature Detector (RTD).

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

Instrument	Serial No.	Cert. No.	Traceable	Due Date
1) Data Acquisition	MY44073381	24LM73	TPA	18 May 2025

2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certification is traceable to the International System of Unit.


Remark : TPA : Technology Promotion Association (Thailand - Japan)

Result of Calibration :- (*) Without Adjustment

Function of UUC* : Temperature Source

Fresh air setting : Close

Environment during calibration		
	Beginning	Finished
Temp. (°C)	28	28
REL.Humid. (%)	56	55
AC Supply (Volt)	224	224

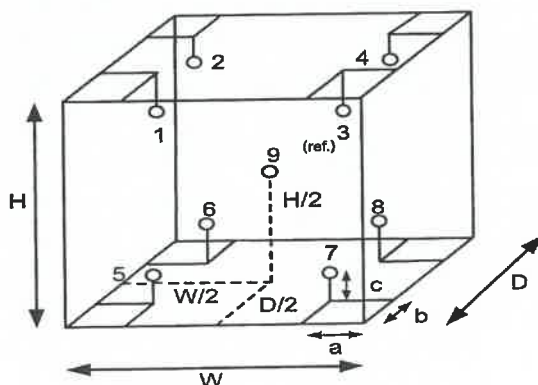

Position :	Ref. Std. ID No.:
1	1RTD-2/1
2	1RTD-2/2
3	22-01RTD-03
4	1RTD-2/4
5	1RTD-2/5
6	1RTD-2/6
7	23-01RTD-07
8	1RTD-2/8
9 (ref.)	23-01RTD-09

Probe Installation Details :

a = 10 cm
 b = 10 cm
 c = 10 cm

Dimension of Chamber :

D = 0.62 m
 W = 1.2 m
 H = 1.2 m
 Capacity = 0.89 m³



Equipment : BOD Incubator
Condition As-Received : Used Item
Reference : 2503-0437OC-2
Result of Calibration :- (*) Without Adjustment
Function of UUC* : Temperature Source
Fresh air setting : Close

Cert. No.: 25TM578
Page : 3 of 3

Calibration Point (°C)	UUC* Setting (°C)	UUC* Reading (°C)	Temperature stability (± °C)	Temperature uniformity (°C)	Overall Variation (°C)	Coverage Factor <i>k</i>
20.0	20.0	19.9	0.49	0.69	1.1	2

Calibration Point (°C)	Measured Temperature (°C)									Uncertainty (± °C)
	Position									
	1	2	3	4	5	6	7	8	9 (ref.)	
20.0	20.025	19.753	20.063	19.839	20.103	20.086	20.152	20.211	19.804	0.69

Average* : The average of 30 values in each position.

Temperature stability : One-half of the greatest maximum difference of measured temperature at any one sensor.

Temperature uniformity : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.

Overall Variation : The Difference of the maximum and minimum measured temperatures throughout observation.

UUC* : Unit Under Calibration

Note : The reported uncertainty of measurement was included stability and excluded uniformity .

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL.0-2717-3000-29 FAX.0-2719-9484



Certificate of Calibration

Cert. No.: 25TM577

Page : 1 of 3

Equipment : BOD Incubator

Manufacturer : ARCO

Model : UR-1320

Serial No. : -

ID No. : UAE.WAO.018/2551

Submitted by : United Analyst and Engineering Consultant Co.,Ltd.
3 Soi Udomsuk 41, Sukhumvit Road,
Bangchak, Phrakhanong,
Bangkok 10260

Location : Lab Floor 2

Received Order : 19 March 2025

Calibration Date : 19 March 2025

Ambient Temperature : $(26 \pm 10) ^\circ\text{C}$

Relative Humidity : $(50 \pm 30) \%$

AC Line Voltage : $(220 \pm 22) \text{ V}$

Calibrated by : Man Pattanapongpaiboon

Kunchit

Approved by :

Approved Signatory

() Chakrit Waewwanjua

() Suwit Imjai

(✓) Kunchit Promprat

Issue Date : 27 March 2025

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

เอกสารไม่ควบคุม



Equipment : BOD Incubator
Condition As-Received : Used Item
Reference : 2503-0437OC-1

Cert. No.: 25TM577
Page : 2 of 3

Procedure Used :-

Calibration were conducted using calibration procedure CP-OT02 based on TLAS G-20 according to direct measurement method with Data Acquisition which connected with Resistance Temperature Detector (RTD).

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

Instrument	Serial No.	Cert. No.	Traceable	Due Date
1) Data Acquisition	MY57013823	24LM71	TPA	12 May 2025

2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certification is traceable to the International System of Unit.


Remark : TPA : Technology Promotion Association (Thailand - Japan)

Result of Calibration :- (*) Without Adjustment

Function of UUC* : Temperature Source

Fresh air setting : Close

Environment during calibration		
	Beginning	Finished
Temp. (°C)	28	28
REL.Humid. (%)	56	55
AC Supply (Volt)	224	224

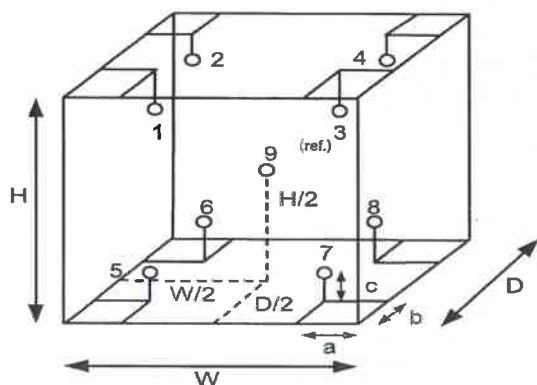

Position :	Ref. Std. ID No.:
1	21-17RTD-01
2	21-17RTD-02
3	17RTD-03
4	24-17RTD-04
5	17RTD-05
6	17RTD-06
7	17RTD-07
8	23-17RTD-08
9 (ref.)	23-17RTD-09

Probe Installation Details :

a = 10 cm
b = 10 cm
c = 10 cm

Dimension of Chamber :

D = 0.62 m
W = 1.2 m
H = 1.2 m
Capacity = 0.89 m³

เอกสารไม่ควบคุม



Equipment : BOD Incubator
Condition As-Received : Used Item
Reference : 2503-0437OC-1
Result of Calibration :- (*) Without Adjustment
Function of UUC* : Temperature Source
Fresh air setting : Close

Cert. No.: 25TM577
Page : 3 of 3

Calibration Point (°C)	UUC* Setting (°C)	UUC* Reading (°C)	Temperature stability (± °C)	Temperature uniformity (°C)	Overall Variation (°C)	Coverage Factor <i>k</i>
20.0	20.0	20.0	0.24	0.54	0.99	2

Calibration Point (°C)	Measured Temperature (°C)									Uncertainty (±°C)
	Position									
	1	2	3	4	5	6	7	8	9 (ref.)	
20.0	20.215	20.192	19.652	19.710	19.710	20.006	19.720	19.810	19.733	0.41

Average* : The average of 30 values in each position.

Temperature stability : One-half of the greatest maximum difference of measured temperature at any one sensor.

Temperature uniformity : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.

Overall Variation : The Difference of the maximum and minimum measured temperatures throughout observation.

UUC* : Unit Under Calibration

Note : The reported uncertainty of measurement was included stability and excluded uniformity .

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

เอกสารไม่ควบคุม



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3 : EQUIPMENT CALIBRATION AND TESTING SERVICES

534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250

TEL. 0-2717-3000 FAX. 0-2719-9484

Certificate of Testing

Cert.No.: 25TW29

Page.: 1 of 2

Equipment :	DO Meter
Manufacturer :	YSI
Model :	5100
Serial No. :	11B 101863
ID No. :	UAE.WAO.004/2554
Received Date :	14 February 2025
Test Date :	17 February 2025
Reference :	2502-0473DSC-1
Submitted by :	United Analyst and Engineering Consultant Co.,Ltd. 3 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Laboratory Condition :	Temperature (25 ± 5) °C Humidity (50 ± 20) %
Test Procedure :	In - house method : CP-CH9 by Comparison Technique with Azide Modification Method
Tested by :	Walalak Sirithean 
Approved by :	Approved Signatory
 () Chakrit Waewwanjua () Ponpan Paipim (✓) Saithip Meangmai	
Issue Date :	18 February 2025

เอกสารไม่ควบคุม



Cert.No.: 25TW29

Page.: 2 of 2

Condition of this result of calibration

1. Reference Standard Instruments :

This certification is traceable to the International System of Unit through the reference standards laboratory of Industrial Calibration Center, Technology Promotion Association (Thailand-Japan).

<u>Instruments</u>	<u>Serial No.</u>	<u>ID No.</u>	<u>Certificate No.</u>	<u>Due Date</u>
1. Burette	-	130BU10	23CG1172	22 Mar 2025
2. Balance	14233821	110RC001	24MM131	04 July 2025

2. Standard Material :-

<u>Material</u>	<u>Manufacturer</u>	<u>Lot.No.</u>	<u>Assay</u>
Sodium Thiosulfate 5-Hydrate AR	KEMAUS	2203162447	99.6%

Result : **Dissolved Oxygen Meter Adjustment With Air 100 %**

Dissolved Oxygen Probe No.: 24F100202

Titration Method (Azide Modification Method) (mg/L)	DO Meter Reading (mg/L)	Standard Deviation (mg/L)
8.22	8.22	0.0055

This report was certified only for the instrument we tested. It is allowable to use for study
Intend to use for advertising and referral purpose is prohibited. This report may not be reproduced
other in full, without written approval of the laboratory

-o0o-

เอกสารไม่ควบคุม

เอกสารไม่ควบคุม

บันทึกผลการตรวจสอบใบรับรองการสอบเทียบ (Verification of Certificate)							
Certificate No. : 25TW29				Equipment : Do Meter			
Brand : YSI				Model : 5100			
Serial No. : 11B 101863				ID No. : UAE.WAO.004/2554			
Calibration results							
Titration Method	Standart Deviation	Do meter Reading	Error%	Correction%	Error Total Error	Judgement	(Total Error < Judgement)
(mg/L)	(mg/L)	(mg/L)	(mg/L)	(mg/L)	(mg/L)	(± mg/L)	(mg/L)
8.22	0.0055	8.22	0.0000	0.0000	0.0	0.02	pass
ผู้บันทึก.....อิศรา.บุญประกอบ.....							
วันที่.....28/02/2025.....							
ผู้ตรวจสอบ.....ผู้ร่าง							
วันที่.....28 ก.พ. 68.....							
หมายเหตุ :							

ทำในชั้น.....

...../.....



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL.0-2717-3000-29 FAX.0-2719-9484



Certificate of Calibration

Cert. No.: 25TM579

Page : 1 of 3

Equipment : Hot Air Oven

Manufacturer : Memmert

Model : UF 55

Serial No. : B212.0411

ID No. : UAE.WAO.005/2556

Submitted by : United Analyst and Engineering Consultant Co.,Ltd.
3 Soi Udomsuk 41, Sukhumvit Road,
Bangchak, Phrakhanong,
Bangkok 10260

Location : Lab Floor 2

Received Order : 19 March 2025


Calibration Date : 19 March 2025

Ambient Temperature : (26 ± 10) °C

Relative Humidity : (50 ± 30) %

AC Line Voltage : (220 ± 22) V

Calibrated by : Man Pattanapongpaiboon

Approved by : 
Approved Signatory

() Chakrit Waewwanjua
() Suwit Imjai
(✓) Kunchit Promprat

Issue Date : 27 March 2025

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

เอกสารไม่ควบคุม



Equipment : Hot Air Oven
 Condition As-Received : Used Item
 Reference : 2503-0437OC-3

Cert. No.: 25TM579

Page : 2 of 3

Procedure Used :-

Calibration were conducted using calibration procedure CP-OT02 based on TLAS G-20 according to direct measurement method with Data Acquisition which connected with Resistance Temperature Detector (RTD) and Thermocouple Type T.

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

Instrument	Serial No.	Cert. No.	Traceable	Due Date
1) Data Acquisition	MY44073381	24LM73	TPA	18 May 2025

2. This certificate is valid only to the item calibrated on date and place of calibration.


3. This certification is traceable to the International System of Unit.

Remark : TPA : Technology Promotion Association (Thailand - Japan)

Result of Calibration :- (*) Without Adjustment

Function of UUC* : Temperature Source

Fresh air setting : Close

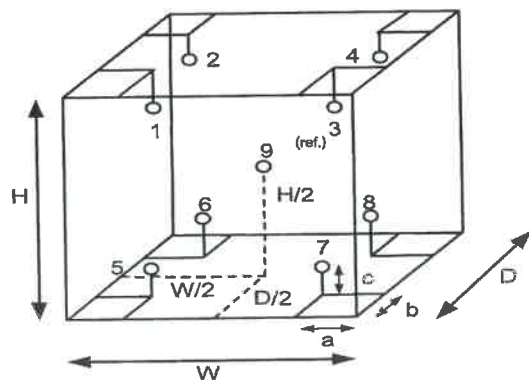

Environment during calibration		
	Beginning	Finished
Temp. (°C)	27	28
REL.Humid. (%)	49	55
AC Supply (Volt)	221	224

Probe Installation Details :

a = 5.0 cm
 b = 5.0 cm
 c = 5.0 cm

Dimension of Chamber :

D = 0.50 m
 W = 0.80 m
 H = 0.75 m
 Capacity = 0.30 m³

Ref. Std. ID No.: @ Calibration Point		
Position :	(120,180) °C	(104) °C
1	23-01TC-01	1RTD-2/1
2	23-01TC-02	1RTD-2/2
3	23-01TC-03	22-01RTD-03
4	23-01TC-04	1RTD-2/4
5	23-01TC-05	1RTD-2/5
6	23-01TC-06	1RTD-2/6
7	23-01TC-07	23-01RTD-07
8	23-01TC-08	1RTD-2/8
9 (ref.)	23-01TC-09	23-01RTD-09

เอกสารไม่ควบคุม



Equipment : Hot Air Oven
Condition As-Received : Used Item
Reference : 2503-0437OC-3
Result of Calibration :- (*) Without Adjustment
Function of UUC* : Temperature Source
Fresh air setting : Close

Cert. No.: 25TM579

Page : 3 of 3

Calibration Point (°C)	UUC* Setting (°C)	UUC* Reading (°C)	Temperature stability (± °C)	Temperature uniformity (°C)	Overall Variation (°C)	Coverage Factor <i>k</i>
104.0	104.0	104.0	0.040	0.43	0.78	2
120.0	120.0	120.0	0.64	1.3	1.6	2
180.0	180.0	180.0	0.49	1.5	1.8	2

Calibration Point (°C)	Measured Temperature (°C)									Uncertainty (± °C)
	Position									
	1	2	3	4	5	6	7	8	9 (ref.)	
104.0	104.335	104.135	104.363	104.317	103.649	103.738	104.179	104.229	104.025	0.42
120.0	119.575	119.366	119.807	119.905	118.994	119.194	119.888	119.994	120.064	1.1
180.0	180.286	179.510	180.401	180.551	179.281	179.463	180.196	180.451	180.374	1.2

Average* : The average of 30 values in each position.

Temperature stability : One-half of the greatest maximum difference of measured temperature at any one sensor.

Temperature uniformity : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.

Overall Variation : The Difference of the maximum and minimum measured temperatures throughout observation.

UUC* : Unit Under Calibration

Note : The reported uncertainty of measurement was included stability and excluded uniformity .

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

FOSS

FOSS South East Asia
3388 Sirinrat Building, 25th – 26th Floor, Unit No. 3388/90,
Rama IV Road, Klongton , Klongtoey, Bangkok, Thailand 10110

Customer Service Report

Report No.: 13852

Date: 25 February 2025

Customer: UAE

Job No.: 11733

Address: Bangkok

Instrument: DT2520 Lift

Serial: 91905060

Start Finish	Travel To Customer (Hrs)		Labour (Hrs)		Travel From Customer (Hrs)	
	07:00		16:00	1hr	17:00	2hrs

Job Type							
Application		Special		Standard			
Distributor	x	Courtesy Visit	x	Installation	x	Training	x
Digital Service	x	PMA Onboarding	x	Quote	x	In House	x
Internal	x	Warranty	x	Repair	x	PM	x
Investigate	x	Sales Support	x	Remote	x	Health Check Visit	x

PMA Type	Smartcare	x	Smartcare Pro	x	Fosscore	x
	Smartcare Advance	x	Fosscore Pro	x	N/A	x

Details of Work / Test				
# PM DT2520 12mo				
- cleaning DT2520, holes				
- check connection cable				
- resistance block 247 Ω				
- test operation				
temperature 250 - 100 $^{\circ}$				
250 - 400 $^{\circ}$ 40 min				
DT meter				
100 100 ± 50				
400 400 ± 20				
- all pass				
Instrument Ready for Use	OK	X	Not OK*	X

Part No:	Batch	Description	Qty
60079730	26.09.2024	FOSS PM test digester 20 pos 12mo	1

I confirm this report is accurate and complete			
Signed FOSS		Signed Customer	Suphakorn P.
Name		Name	

Email:		Customer Contact.:	
--------	--	--------------------	--

*Remark:

เอกสารไม่ควมารถใช้

Please scan QR code



FOSS

FOSS South East Asia
3388 Sirinrat Building, 25th – 26th Floor, Unit No. 3388/90,
Rama IV Road, Klongton , Klongtoey, Bangkok, Thailand 10110

Customer Service Report

Report No.: 13319

Date: Jan 27, 2025

Customer: UAE

Job No.: 11675

Address: Bangkok

Instrument: KT200

Serial: 91790524

Start Finish	Travel To Customer (Hrs)		Labour (Hrs)		Travel From Customer (Hrs)	
	09.00	1	10.00	3	-	-

Job Type					
Application		Special		Standard	
Distributor	x	Courtesy Visit	x	Installation	x
Digital Service	x	PMA Onboarding	x	Quote	x
Internal	x	Warranty	x	Repair	x
Investigate	x	Sales Support	x	Remote	x

PMA Type	Smartcare	x	Smartcare Pro	x	Fosscore	x
	Smartcare Advance	x	Fosscore Pro	x	N/A	x

Details of Work / Test			
- PM - + Visual Check - No leak - have damage on heater & main switch - replace heater - 10% main switch intervention via - replace PM kit & 1 set - Function Check - Power ON / OFF - Alkali - Steam - Condenser			
Instrument Ready for Use		OK	Not OK*

Part No:	Batch	Description	Qty
10069965	11-06-2024	FOSS PM kit KT200 heater Analyser / 2100	1
10003512	29.03.2024	Heating element Steam	1
15630111	19.10.2022	Switch R595kmt + 2 FA	1

I confirm this report is accurate and complete			
Signed FOSS		Signed Customer	
Name		Name	

Email:	Customer Contact.:
	เอกสารไม่ควบคุม

*Remark:

FOSS

Customer Service Report

FOSS South East Asia

3388 Sirinrat Building, 25th – 26th Floor, Unit No. 3388/90,
Rama IV Road, Klongton, Klongtoey, Bangkok, Thailand 10110

Report No.:

13854

Date:

24 February 2025

Customer:

UAE

Job No.:

11735

Address:

Bangkok

Instrument:

KT8100

Serial:

91889052

Start
Finish

Travel To Customer (Hrs)

07:00

09:00

2hrs

Labour (Hrs)

09:00-12:00

13:00-14:00

5hrs

Travel From Customer (Hrs)

15:00

17:00

Job Type							
Application		Special		Standard		Standard	
Distributor	x	Courtesy Visit	x	Installation	x	Training	x
Digital Service	x	PMA Onboarding	x	Quote	x	In House	x
Internal	x	Warranty	x	Repair	x	PM	x
Investigate	x	Sales Support	x	Remote	x	Health Check Visit	x

PMA Type	Smartcare	x	Smartcare Pro	x	Fosscore	x
	Smartcare Advance	x	Fosscore Pro	x	N/A	x

Details of Work / Test


PM KT8100 12MO

- test before PM
- cleaning KT8100, 36 mo replace
- flushing Alkali pump
- test operation
 - Dilution 80 - 80 ml
 - Distillation 5 min 150-170ml
 - Alkali 50-50ml
 - All pass

Instrument Ready for Use	OK	x	Not OK*	x
--------------------------	----	---	---------	---

Part No:	Batch	Description	Qty
60031810	08-01-2024	FOSS PM test KT809 6200 36MO	1

I confirm this report is accurate and complete

Signed FOSS		Signed Customer	Suphakorn P.
Name		Name	

Email:

Customer Contact.:

*Remark:

เอกสารไม่ควรถูกแก้ไข

Please scan QR code





TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL.0-2717-3000-29 FAX.0-2719-9484



Certificate of Calibration

Cert.No.: 25CH408

Page.: 1 of 3

Equipment : pH Meter
Manufacturer : EcoSense
Model : pH100A
Serial No. : JC04744
ID No. : UAE.EFM.058/2566 (EFM.pH.01/66)
Condition As-Received: Used Item
Received Date : 01 April 2025
Calibration Date : 03 April 2025
Reference : 2504-0031WSC-1
Submitted by : United Analyst and Engineering Consultant Co.,Ltd.
3 Soi Udomsuk 41, Sukhumvit Road, Bangchak,
Phrakhanong, Bangkok 10260

Ambient Temperature : (25 $\pm$ 2.5) °C
Relative Humidity : (50 $\pm$ 15) %
Calibration Procedure : In - house method :
- CP-CH5 by direct measurement with DC voltage
standard and direct measurement with
certified reference material (CRM)
- CP-CH8 by comparison with temperature standard

Calibrated by : Walalak Sirithean

Approved by :

Approved Signatory

() Chakrit Waewwanjua
() Ponpan Paipim
(✓) Saithip Meangmai

Issue Date : 4 April 2025

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

เอกสารไม่ควบคุม



Cert.No.: 25CH408

Page.: 2 of 3

Condition of this calibration result

1. Reference Standard Instrument

<u>Instrument</u>	<u>Serial No.</u>	<u>ID No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
1) Document Process Calibrator	54030049	130RC116	24E2759	25 Aug 2025
2) Ref. Standard Thermometer	4982054	110RC044	24I757	14 July 2025

- This Certification is traceable to SI Through Technology Promotion Association (Thailand - Japan)

- 2. Certified Reference Materials** :The measurement results are traceable to SI through Hach Lenge GmbH Ltd.,
Deutsche Akkreditierungsstelle, Accredited No.D-RM-15184-01-00
:The measurement results are traceable to SI through CPA chem Ltd.,
ANSI-ASQ National Accreditation Board, Accredited No. AR-1835

<u>Buffer Solution</u>	<u>Manufacturer</u>	<u>Lot No.</u>	<u>Exp. date</u>
pH 4.007	CPA chem	1066665	18 Jan 2027
pH 6.999	Hach Lenge GmbH	C03220	29 Oct 2026
pH 10.010	CPA chem	1066669	18 Jan 2026

- 3. This certificate is valid only to the item calibrated on date and place of calibration.**

Calibration Results

Function : mV Measurement

Performing standard curve by Document Process Calibrator at pH (4,7)(7,10)

Unit Under Calibration	Nominal Value	Standard Voltage Input	Actual Reading		Uncertainty of Measurement (±mV)	Coverage factor <i>k</i>
	pH	mV	mV	pH		
pH Meter S/N.: JC04744	4.00	177.48	177	4.01	0.58	2.00
	7.00	0.00	0	7.00	0.58	2.00
	7.00	0.00	0	7.00	0.58	2.00
	10.00	-177.48	-177	10.01	0.58	2.00

เอกสารไม่ควบคุม



Cert.No.: 25CH408

Page.: 3 of 3

Calibration Results

Function : pH Measurement

Performing three buffers standard curve by using buffer nominal pH (4,7)(7,10)

Unit Under Calibration	Standard pH Buffer Solution	Actual pH Reading	Actual mV Reading (mV)	Uncertainty of pH Measurement ($\pm$)	Coverage factor k
pH Electrode S/N.: 240710SIA605377	4.007	4.01	173	0.0085	2.05
	6.999	7.00	-2	0.0095	2.00
	6.999	7.00	-2	0.0085	2.00
	10.010	10.00	-176	0.0095	2.00

Function : Temperature Measurement

(*) Without adjustment

This equipment was connected with Temperature Probe;

- Model : -
- Serial No. : 240710SIA605377

Dimension of probe

- Length : 110 mm.
- Diameter : 12 mm.
- Immersion Depth : 100 mm.

Calibration Point (°C)	Standard Temperature (°C)	UUC* Reading (°C)	Error (°C)	Uncertainty of measurement ($\pm$ °C)	Coverage factor k
15.0	15.000	14.9	-0.100	0.13	2.00
30.0	30.001	29.9	-0.101	0.13	2.00
45.0	45.002	45.0	-0.002	0.13	2.00

Remark - UUC* = Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k , providing a level of confidence of approximately 95 %.

-o0o-

เอกสารไม่ควบคุม



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL.0-2717-3000-29 FAX.0-2719-9484



Certificate of Calibration

Cert.No.: 24CH1596

Page.: 1 of 3

Equipment : pH Meter
Manufacturer : Horiba
Model : LAQUA-PH210
Serial No. : HA9M0046
ID No. : UAE.EFM.001/2563(EFM.pH.01/63)
Condition As-Received: Used Item
Received Date : 24 December 2024
Calibration Date : 26 December 2024
Reference : 2412-0601WSC-1
Submitted by : United Analyst and Engineering Consultant Co.,Ltd.
3 Soi Udomsuk 41, Sukhumvit Road,
Bangchak, Phrakhanong, Bangkok 10260

Ambient Temperature : (25 ± 2.5) °C
Relative Humidity : (50 ± 15) %
Calibration Procedure : In - house method :
- CP-CH5 by direct measurement with DC voltage
standard and direct measurement with
certified reference material (CRM)
- CP-CH8 by comparison with temperature standard

Calibrated by : Warakorn Lerngagtrakul

Approved by : _____
Approved Signatory

() Pornthippa Tameyakul
() Ponpan Paipim
(✓) Saithip Meangmai
Issue Date : 27 December 2024

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

เอกสารไม่ควบคุม

 ☒ PASS ☐ NOT PASS	
Remarks	Temp ± 0.5 (std. thermometer)
	mV ± 30 (std. voltage input)
	pH ± 0.05 (std. buffer solution)
<u> </u>	<u> </u>
(<u> </u>)	(<u> </u>)
Verify	Approve

6/1/69

เอกสารไม่ควบคุม



Cert.No.: 24CH1596

Page.: 2 of 3

Condition of this calibration result

1. Reference Standard Instrument

<u>Instrument</u>	<u>Serial No.</u>	<u>ID No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
1)Document Process Calibrator	54030049	130RC116	24E2759	25 Aug 2025
2)Ref. Standard Thermometer	4982054	110RC044	24I757	14 July 2025

- This Certification is traceable to SI Through Technology Promotion Association (Thailand - Japan)

2. Certified Reference Materials :The measurement results are traceable to SI through Hach Lenge GmbH Ltd.,

Deutsche Akkreditierungsstelle, Accredited No.D-RM-15184-01-00

:The measurement results are traceable to SI through CPA chem Ltd.,

ANSI-ASQ National Accreditation Board, Accredited No. AR-1835

<u>Buffer Solution</u>	<u>Manufacturer</u>	<u>Lot No.</u>	<u>Exp. date</u>
pH 4.008	CPA chem	1034203	27 Sep 2026
pH 7.000	Hach Lenge GmbH	C03185	09 July 2026
pH 10.010	CPA chem	1034205	27 Sep 2025

3. This certificate is valid only to the item calibrated on date and place of calibration.

Calibration Results

Function : mV Measurement

Performing standard curve by Document Process Calibrator at pH (4,7)(7,10)

Unit Under Calibration	Nominal Value	Standard Voltage Input	Actual Reading		Uncertainty of Measurement (±mV)	Coverage factor <i>k</i>
	pH	mV	mV	pH		
pH Meter S/N.: HA9M0046	4.00	177.48	177.6	4.01	0.058	2.00
	7.00	0.00	0.2	7.00	0.058	2.00
	7.00	0.00	0.2	7.00	0.058	2.00
	10.00	-177.48	-177.1	10.01	0.058	2.00

เอกสารไม่ควบคุม



Cert.No.: 24CH1596

Page.: 3 of 3

Calibration Results

Function : pH Measurement

Performing three buffers standard curve by using buffer nominal pH (4,7)(7,10)

Unit Under Calibration	Standard pH Buffer Solution	Actual pH Reading	Actual mV Reading (mV)	Uncertainty of pH Measurement ($\pm$)	Coverage factor k
pH Electrode S/N.: -	4.008	4.01	184.8	0.0071	2.00
	7.000	6.99	9.1	0.0092	2.00
	7.000	7.00	9.1	0.0085	2.00
	10.010	10.01	-164.5	0.011	2.07

Function : Temperature Measurement

(*) Without adjustment

This equipment was connected with Temperature Probe;

- Model : _____ -

- Serial No. : _____ -

Dimension of probe

- Length : _____ 112 mm.

- Diameter : _____ 16 mm.

- Immersion Depth : _____ 100 mm.

Calibration Point (°C)	Standard Temperature (°C)	UUC* Reading (°C)	Error (°C)	Uncertainty of measurement ($\pm$ °C)	Coverage factor k
15.0	15.001	15.0	-0.001	0.13	2.00
30.0	30.003	30.0	-0.003	0.13	2.00
45.0	45.004	45.0	-0.004	0.13	2.00

Remark - UUC* = Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k , providing a level of confidence of approximately 95 %.

-o0o-

เอกสารไม่ควบคุม



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL.0-2717-3000-29 FAX.0-2719-9484



Certificate of Calibration

Cert.No.: 25CH586

Page.: 1 of 3

Equipment :	pH Meter
Manufacturer :	Horiba
Model :	LAQUA-PH210
Serial No. :	HA9M0048
ID No. :	UAE.EFM.003/2563(EFM.pH.03/63)
Condition As-Received:	Used Item
Received Date :	20 May 2025
Calibration Date :	21 May 2025
Reference :	2505-0602WSC-1
Submitted by :	United Analyst and Engineering Consultant Co.,Ltd. 3 Soi Udomsuk 41, Sukhumvit Road, Bangkok, Phrakhanong, Bangkok 10260
Ambient Temperature :	(25 ± 2.5) °C
Relative Humidity :	(50 ± 15) %
Calibration Procedure :	In - house method : - CP-CH5 by direct measurement with DC voltage standard and direct measurement with certified reference material (CRM) - CP-CH8 by comparison with temperature standard
Calibrated by :	Walalak Sirithean
Approved by :	 Approved Signatory
() Chakrit Waewwanjua	
() Ponpan Paipim	
(✓) Saithip Meangmai	
Issue Date :	23 May 2025

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

เอกสารไม่ควบคุม



Cert.No.: 25CH586
Page.: 2 of 3

Condition of this calibration result

1. Reference Standard Instrument

<u>Instrument</u>	<u>Serial No.</u>	<u>ID No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
1) Document Process Calibrator	54030049	130RC116	24E2759	25 Aug 2025
2) Ref. Standard Thermometer	4982054	110RC044	24I757	14 July 2025

- This measurement result is traceable to SI through Technology Promotion Association (Thailand - Japan)

2. Certified Reference Materials :The measurement results are traceable to SI through Hach Lenge GmbH Ltd.,
Deutsche Akkreditierungsstelle, Accredited No.D-RM-15184-01-00
:The measurement results are traceable to SI through CPA chem Ltd.,
ANSI-ASQ National Accreditation Board, Accredited No. AR-1835

<u>Buffer Solution</u>	<u>Manufacturer</u>	<u>Lot No.</u>	<u>Exp. date</u>
pH 4.007	CPA chem	1066665	18 Jan 2027
pH 7.000	Hach Lenge GmbH	C03232	02 Dec 2026
pH 10.010	CPA chem	1066669	18 Jan 2026

3. This certificate is valid only to the item calibrated on date and place of calibration.

Calibration Results

Function : mV Measurement

Performing standard curve by Document Process Calibrator at pH (4,7)(7,10)

Unit Under Calibration	Nominal Value	Standard Voltage Input	Actual Reading		Uncertainty of Measurement (±mV)	Coverage factor k
	pH	mV	mV	pH		
pH Meter S/N.: HA9M0048	4.00	177.48	177.4	4.01	0.058	2.00
	7.00	0.00	0.0	7.00	0.058	2.00
	7.00	0.00	0.0	7.00	0.058	2.00
	10.00	-177.48	-177.5	10.01	0.058	2.00

เอกสารไม่ควบคุม



Cert.No.: 25CH586

Page.: 3 of 3

Calibration Results

Function : pH Measurement

Performing three buffers standard curve by using buffer nominal pH (4,7)(7,10)

Unit Under Calibration	Standard pH Buffer Solution	Actual pH Reading	Actual mV Reading (mV)	Uncertainty of pH Measurement ($\pm$)	Coverage factor k
pH Electrode S/N.: Q9AD0211	4.007	4.01	169.9	0.0071	2.00
	7.000	7.00	-3.5	0.0096	2.00
	7.000	7.00	-3.0	0.0092	2.00
	10.010	10.01	-175.3	0.0096	2.00

Function : Temperature Measurement

(*) Without adjustment

This equipment was connected with Temperature Probe;

- Model : 9652-10D

- Serial No. : Q9AD0211

Dimension of probe

- Length : 103 mm.

- Diameter : 16 mm.

- Immersion Depth : 80 mm.

Calibration Point ($^{\circ}\text{C}$)	Standard Temperature ($^{\circ}\text{C}$)	UUC* Reading ($^{\circ}\text{C}$)	Error ($^{\circ}\text{C}$)	Uncertainty of measurement ($\pm$ $^{\circ}\text{C}$)	Coverage factor k
15.0	15.002	15.0	-0.002	0.13	2.00
30.0	29.999	30.0	0.001	0.13	2.00
45.0	45.001	45.0	-0.001	0.13	2.00

Remark - UUC* = Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k , providing a level of confidence of approximately 95 %.

-o0o-

เอกสารไม่ควบคุม



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL.0-2717-3000-29 FAX.0-2719-9484



Certificate of Calibration

Cert.No.: 24CH1597

Page.: 1 of 3

Equipment :	pH Meter
Manufacturer :	Horiba
Model :	LAQUA-PH210
Serial No. :	HA0A0005
ID No. :	UAE.EFM.004/2563(EFM.pH.04/63)
Condition As-Received:	Used Item
Received Date :	24 December 2024
Calibration Date :	26 December 2024
Reference :	2412-0601WSC-2
Submitted by :	United Analyst and Engineering Consultant Co.,Ltd. 3 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Ambient Temperature :	(25 ± 2.5) °C
Relative Humidity :	(50 ± 15) %
Calibration Procedure :	In - house method : - CP-CH5 by direct measurement with DC voltage standard and direct measurement with certified reference material (CRM) - CP-CH8 by comparison with temperature standard
Calibrated by :	Warakorn Lerngagtrakul
Approved by :	 Approved Signatory
() Pornthippa Tameyakul	
() Ponpan Paipim	
(✓) Saithip Meangmai	
Issue Date :	27 December 2024

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

เอกสารไม่ควบคุม



Cert.No.: 24CH1597

Page.: 2 of 3

Condition of this calibration result

1. Reference Standard Instrument

<u>Instrument</u>	<u>Serial No.</u>	<u>ID No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
1) Document Process Calibrator	54030049	130RC116	24E2759	25 Aug 2025
2) Ref. Standard Thermometer	4982054	110RC044	24I757	14 July 2025

- This Certification is traceable to SI Through Technology Promotion Association (Thailand - Japan)

2. Certified Reference Materials :The measurement results are traceable to SI through Hach Lenge GmbH Ltd.,

Deutsche Akkreditierungsstelle, Accredited No.D-RM-15184-01-00

:The measurement results are traceable to SI through CPA chem Ltd.,

ANSI-ASQ National Accreditation Board, Accredited No. AR-1835

<u>Buffer Solution</u>	<u>Manufacturer</u>	<u>Lot No.</u>	<u>Exp. date</u>
pH 4.008	CPA chem	1034203	27 Sep 2026
pH 7.000	Hach Lenge GmbH	C03185	09 July 2026
pH 10.010	CPA chem	1034205	27 Sep 2025

3. This certificate is valid only to the item calibrated on date and place of calibration.

Calibration Results

Function : mV Measurement

Performing standard curve by Document Process Calibrator at pH (4,7)(7,10)

Unit Under Calibration	Nominal Value	Standard Voltage Input	Actual Reading		Uncertainty of Measurement (±mV)	Coverage factor k
	pH	mV	mV	pH		
pH Meter S/N.: HAOA0005	4.00	177.48	177.4	4.01	0.058	2.00
	7.00	0.00	0.1	7.00	0.058	2.00
	7.00	0.00	0.1	7.00	0.058	2.00
	10.00	-177.48	-177.2	10.01	0.058	2.00

เอกสารไม่ควบคุม



Cert.No.: 24CH1597

Page.: 3 of 3

Calibration Results

Function : pH Measurement

Performing three buffers standard curve by using buffer nominal pH (4,7)(7,10)

Unit Under Calibration	Standard pH Buffer Solution	Actual pH Reading	Actual mV Reading (mV)	Uncertainty of pH Measurement ($\pm$)	Coverage factor k
pH Electrode S/N.: -	4.008	4.01	177.2	0.0079	2.00
	7.000	7.00	2.2	0.0092	2.00
	7.000	7.00	2.2	0.0085	2.00
	10.010	10.01	-170.9	0.0095	2.00

Function : Temperature Measurement

(*) Without adjustment

This equipment was connected with Temperature Probe;

- Model : _____ -

- Serial No. : _____ -

Dimension of probe

- Length : _____ 112 mm.

- Diameter : _____ 16 mm.

- Immersion Depth : _____ 100 mm.

Calibration Point (°C)	Standard Temperature (°C)	UUC* Reading (°C)	Error (°C)	Uncertainty of measurement ($\pm$ °C)	Coverage factor k
15.0	15.003	15.0	-0.003	0.13	2.00
30.0	30.001	30.0	-0.001	0.13	2.00
45.0	45.002	45.0	-0.002	0.13	2.00

Remark - UUC* = Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k , providing a level of confidence of approximately 95 %.

-o0o-

เอกสารไม่ควบคุม



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL.0-2717-3000-29 FAX.0-2719-9484



Certificate of Calibration

Cert.No.: 25CH354

Page.: 1 of 3

Equipment : pH Meter
Manufacturer : Horiba
Model : LAQUA-PH210
Serial No. : HA9M0047
ID No. : UAE.EFM.005/2563 (EFM.pH.05/63)
Condition As-Received: Used Item
Received Date : 18 March 2025
Calibration Date : 20 March 2025
Reference : 2503-0612WSC-2
Submitted by : United Analyst and Engineering Consultant Co.,Ltd.
3 Soi Udomsuk 41, Sukhumvit Road, Bangchak,
Phrakhanong, Bangkok 10260

Ambient Temperature : (25 ± 2.5) °C
Relative Humidity : (50 ± 15) %
Calibration Procedure : In - house method :
- CP-CH5 by direct measurement with DC voltage
standard and direct measurement with
certified reference material (CRM)
- CP-CH8 by comparison with temperature standard

Calibrated by : Uthen Kankawi

Approved by : _____
Approved Signatory

() Chakrit Waewwanjua
() Ponpan Paipim
(✓) Saithip Meangmai

Issue Date : 20 March 2025

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

เอกสารไม่ควบคุม



Cert.No.: 25CH354

Page.: 2 of 3

Condition of this calibration result

1. Reference Standard Instrument

<u>Instrument</u>	<u>Serial No.</u>	<u>ID No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
1) Document Process Calibrator	43160066	130RC092	24E1320	22 Apr 2025
2) Ref. Standard Thermometer	4982054	110RC044	24I757	14 Jul 2025

- This Certification is traceable to SI Through Technology Promotion Association (Thailand - Japan)

- 2. Certified Reference Materials** :The measurement results are traceable to SI through Hach Lenge GmbH Ltd.,
Deutsche Akkreditierungsstelle, Accredited No.D-RM-15184-01-00
: The measurement results are traceable to SI through CPA chem Ltd.,
ANSI-ASQ National Accreditation Board, Accredited No. AR-1835

<u>Buffer Solution</u>	<u>Manufacturer</u>	<u>Lot No.</u>	<u>Exp. date</u>
pH 4.007	CPA chem	1066665	18 Jan 2027
pH 6.999	Hach Lenge GmbH	C03220	29 Oct 2026
pH 10.010	CPA chem	1066669	18 Jan 2026

- 3. This certificate is valid only to the item calibrated on date and place of calibration.**

Calibration Results

Function : mV Measurement

Performing standard curve by Document Process Calibrator at pH (4,7)(7,10)

Unit Under Calibration	Nominal Value	Standard Voltage Input	Actual Reading		Uncertainty of Measurement (±mV)	Coverage factor k
	pH	mV	mV	pH		
pH Meter S/N.: HA9M0047	4.00	177.48	177.7	4.01	0.058	2.00
	7.00	0.00	0.3	7.01	0.058	2.00
	7.00	0.00	0.3	7.01	0.058	2.00
	10.00	-177.48	-176.8	10.01	0.058	2.00

เอกสารไม่ควบคุม



Cert.No.: 25CH354

Page.: 3 of 3

Calibration Results

Function : pH Measurement

Performing three buffers standard curve by using buffer nominal pH (4,7)(7,10)

Unit Under Calibration	Standard pH Buffer Solution	Actual pH Reading	Actual mV Reading (mV)	Uncertainty of pH Measurement ($\pm$)	Coverage factor k
pH Electrode S/N.: -	4.007	4.01	168.5	0.011	2.13
	6.999	7.00	-5.9	0.012	2.09
	6.999	7.00	-6.1	0.011	2.07
	10.010	10.02	-176.7	0.010	2.00

Function : Temperature Measurement

(*) Without adjustment

This equipment was connected with Temperature Probe;

- Model : -

- Serial No. : -

Dimension of probe

- Length : 103 mm.

- Diameter : 16 mm.

- Immersion Depth : 90 mm.

Calibration Point (°C)	Standard Temperature (°C)	UUC* Reading (°C)	Error (°C)	Uncertainty of measurement ($\pm$ °C)	Coverage factor k
15.0	15.005	15.0	-0.005	0.13	2.00
30.0	30.007	30.0	-0.007	0.13	2.00
45.0	44.995	44.9	-0.095	0.13	2.00

Remark - UUC* = Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k , providing a level of confidence of approximately 95 %.

-o0o-

เอกสารไม่ควบคุม



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL.0-2717-3000-29 FAX.0-2719-9484



Certificate of Calibration

Cert.No.: 25CH261

Page.: 1 of 3

Equipment : pH Meter
Manufacturer : Horiba
Model : LAQUA-PH210
Serial No. : HA0C0025
ID No. : UAE.EFM.117/2563(EFM.pH.07/63)
Condition As-Received: Used Item
Received Date : 25 February 2025
Calibration Date : 26 to 28 February 2025
Reference : 2502-0783WSC-1
Submitted by : United Analyst and Engineering Consultant Co.,Ltd.
3 Soi Udomsuk 41, Sukhumvit Road,
Bangchak, Phrakhanong, Bangkok 10260
Ambient Temperature : (25 ± 2.5) °C
Relative Humidity : (50 ± 15) %
Calibration Procedure : In - house method :
- CP-CH5 by direct measurement with DC voltage
standard and direct measurement with
certified reference material (CRM)
- CP-CH8 by comparison with temperature standard
Calibrated by : Warakorn Lerngagtrakul
Approved by :

Approved Signatory

☐ Chakrit Waewwanjua
☐ Ponpan Paipim
☒ Saithip Meangmai

Issue Date : 28 February 2025

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

เอกสารไม่ควบคุม



Cert.No.: 25CH261

Page.: 2 of 3

Condition of this calibration result

1. Reference Standard Instrument

<u>Instrument</u>	<u>Serial No.</u>	<u>ID No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
1)Document Process Calibrator	54030049	130RC116	24E2759	25 Aug 2025
2)Ref. Standard Thermometer	4982054	110RC044	24I757	14 July 2025

- This Certification is traceable to SI Through Technology Promotion Association (Thailand - Japan)

- 2. Certified Reference Materials** : The measurement results are traceable to SI through Hach Lenge GmbH Ltd.,
Deutsche Akkreditierungsstelle, Accredited No.D-RM-15184-01-00
: The measurement results are traceable to SI through CPA chem Ltd.,
ANSI-ASQ National Accreditation Board, Accredited No. AR-1835

<u>Buffer Solution</u>	<u>Manufacturer</u>	<u>Lot No.</u>	<u>Exp. date</u>
pH 4.007	CPA chem	1066665	18 Jan 2027
pH 6.999	Hach Lenge GmbH	C03220	29 Oct 2026
pH 10.010	CPA chem	1066669	18 Jan 2026

- 3. This certificate is valid only to the item calibrated on date and place of calibration.**

Calibration Results

Function : mV Measurement

Performing standard curve by Document Process Calibrator at pH (4,7)(7,10)

Unit Under Calibration	Nominal Value	Standard Voltage Input	Actual Reading		Uncertainty of Measurement (±mV)	Coverage factor <i>k</i>
	pH	mV	mV	pH		
pH Meter S/N.: HA0C0025	4.00	177.48	177.5	4.01	0.058	2.00
	7.00	0.00	0.0	7.02	0.058	2.00
	7.00	0.00	0.0	7.02	0.058	2.00
	10.00	-177.48	-177.5	10.01	0.058	2.00

เอกสารไม่ควบคุม



Cert.No.: 25CH261

Page.: 3 of 3

Calibration Results

Function : pH Measurement

Performing three buffers standard curve by using buffer nominal pH (4,7)(7,10)

Unit Under Calibration	Standard pH Buffer Solution	Actual pH Reading	Actual mV Reading (mV)	Uncertainty of pH Measurement ($\pm$)	Coverage factor k
pH Electrode S/N.: Q9AG0214	4.007	4.01	178.4	0.0071	2.00
	6.999	7.00	4.1	0.0092	2.00
	6.999	7.00	3.0	0.0095	2.00
	10.010	10.01	-169.8	0.0092	2.00

Function : Temperature Measurement

(*) Without adjustment

This equipment was connected with Temperature Probe;

- Model : 9652-10D

- Serial No. : Q9AG0214

Dimension of probe

- Length : 110 mm.

- Diameter : 16 mm.

- Immersion Depth : 80 mm.

Calibration Point (°C)	Standard Temperature (°C)	UUC* Reading (°C)	Error (°C)	Uncertainty of measurement ($\pm$ °C)	Coverage factor k
15.0	15.002	15.0	-0.002	0.13	2.00
30.0	30.003	30.0	-0.003	0.13	2.00
45.0	45.002	44.9	-0.102	0.13	2.00

Remark - UUC* = Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k , providing a level of confidence of approximately 95 %.

-o0o-

เอกสารไม่ควบคุม

List of Instruments Certification for Water Quality Analysis

No.	Instrument/Equipment	Parameter	Manufacturer	Model/Serial No.	Calibrator	Certification No.	Date of Calibration	Due date of Calibration	Remark
Water									
1	pH Meter	pH	Ecosence	pH1100A JC04740	Technology Promotion Association (Thailand-Japan)	25CH264	26 Feb 25	25 Feb 26	-



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL.0-2717-3000-29 FAX.0-2719-9484



Certificate of Calibration

Cert.No.: 25CH264

Page.: 1 of 3

Equipment :	pH Meter
Manufacturer :	EcoSence
Model :	pH100A
Serial No. :	JC04740
ID No. :	UAE.EFM.062/2566(EFM.pH.05/66)
Condition As-Received:	Used Item
Received Date :	25 February 2025
Calibration Date :	26 to 28 February 2025
Reference :	2502-0783WSC-4
Submitted by :	United Analyst and Engineering Consultant Co.,Ltd. 3 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Ambient Temperature :	(25 ± 2.5) °C
Relative Humidity :	(50 ± 15) %
Calibration Procedure :	In - house method : - CP-CH5 by direct measurement with DC voltage standard and direct measurement with certified reference material (CRM) - CP-CH8 by comparison with temperature standard
Calibrated by :	Warakorn Lerngagtrakul
Approved by :	Approved Signatory
() Chakrit Waewwanjua	
() Ponpan Paipim	
(✓) Saithip Meangmai	
Issue Date :	28 February 2025

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

เอกสารไม่ควบคุม



Cert.No.: 25CH264

Page.: 2 of 3

Condition of this calibration result

1. Reference Standard Instrument

<u>Instrument</u>	<u>Serial No.</u>	<u>ID No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
1)Document Process Calibrator	54030049	130RC116	24E2759	25 Aug 2025
2)Ref. Standard Thermometer	4982054	110RC044	24I757	14 July 2025

- This Certification is traceable to SI Through Technology Promotion Association (Thailand - Japan)

- 2. Certified Reference Materials** :The measurement results are traceable to SI through Hach Lenge GmbH Ltd.,
Deutsche Akkreditierungsstelle, Accredited No.D-RM-15184-01-00
: The measurement results are traceable to SI through CPA chem Ltd.,
ANSI-ASQ National Accreditation Board, Accredited No. AR-1835

<u>Buffer Solution</u>	<u>Manufacturer</u>	<u>Lot No.</u>	<u>Exp. date</u>
pH 4.007	CPA chem	1066665	18 Jan 2027
pH 6.999	Hach Lenge GmbH	C03220	29 Oct 2026
pH 10.010	CPA chem	1066669	18 Jan 2026

- 3. This certificate is valid only to the item calibrated on date and place of calibration.**

Calibration Results

Function : mV Measurement

Performing standard curve by Document Process Calibrator at pH (4,7)(7,10)

Unit Under Calibration	Nominal Value	Standard Voltage Input	Actual Reading		Uncertainty of Measurement (±mV)	Coverage factor <i>k</i>
	pH	mV	mV	pH		
pH Meter S/N.: JC04740	4.00	177.48	177	4.01	0.58	2.00
	7.00	0.00	0	7.00	0.58	2.00
	7.00	0.00	0	7.00	0.58	2.00
	10.00	-177.48	-177	10.01	0.58	2.00

เอกสารไม่ควบคุม



Cert.No.: 25CH264

Page.: 3 of 3

Calibration Results

Function : pH Measurement

Performing three buffers standard curve by using buffer nominal pH (4,7)(7,10)

Unit Under Calibration	Standard pH Buffer Solution	Actual pH Reading	Actual mV Reading (mV)	Uncertainty of pH Measurement ($\pm$)	Coverage factor k
pH Electrode S/N.: 240710SIA605377	4.007	4.01	173	0.0079	2.00
	6.999	7.01	-2	0.0085	2.00
	6.999	7.01	-2	0.0085	2.00
	10.010	10.01	-177	0.0092	2.00

Function : Temperature Measurement

(*) Without adjustment

This equipment was connected with Temperature Probe;

- Model : -

- Serial No. : 240710SIA605377

Dimension of probe

- Length : 112 mm.

- Diameter : 12 mm.

- Immersion Depth : 100 mm.

Calibration Point (°C)	Standard Temperature (°C)	UUC* Reading (°C)	Error (°C)	Uncertainty of measurement ($\pm$ °C)	Coverage factor k
15.0	15.004	14.7	-0.304	0.13	2.00
30.0	30.002	29.8	-0.202	0.13	2.00
45.0	45.003	44.8	-0.203	0.13	2.00

Remark - UUC* = Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k , providing a level of confidence of approximately 95 %.

-o0o-

เอกสารไม่ควบคุม