

ภาคผนวกที่ 5

เอกสารสอบเทียบความถูกต้องของเครื่องมือ

เอกสารแนบ 5-1	เอกสารสอบเทียบเครื่องมือการตรวจวัดคุณภาพอากาศในบรรยากาศ
เอกสารแนบ 5-2	เอกสารสอบเทียบเครื่องมือการตรวจวัดคุณภาพอากาศจากปล่อง
เอกสารแนบ 5-3	เอกสารสอบเทียบเครื่องมือการตรวจวัดระดับเสียงในบรรยากาศ
เอกสารแนบ 5-4	เอกสารสอบเทียบเครื่องมือการตรวจวิเคราะห์คุณภาพน้ำทิ้ง
เอกสารแนบ 5-5	เอกสารสอบเทียบเครื่องมือการตรวจวิเคราะห์คุณภาพน้ำใต้ดิน
เอกสารแนบ 5-6	เอกสารสอบเทียบเครื่องมือการตรวจวัดคุณภาพอากาศในสถานประกอบการ
เอกสารแนบ 5-7	เอกสารสอบเทียบเครื่องมือการตรวจวัดระดับเสียงในสถานประกอบการ
เอกสารแนบ 5-8	เอกสารสอบเทียบเครื่องมือการตรวจวัดปริมาณเสียงสะสมติดตัวพนักงาน
เอกสารแนบ 5-9	เอกสารสอบเทียบเครื่องมือการตรวจวัดแสงสว่างในสถานประกอบการ
เอกสารแนบ 5-10	เอกสารสอบเทียบเครื่องมือการตรวจวัดระดับความร้อนในสถานประกอบการ

ตารางสรุปรายการเอกสารการสอบเทียบความถูกต้องของเครื่องมือเก็บตัวอย่างและตรวจวิเคราะห์

รายการตรวจวัด	เครื่องมือเก็บตัวอย่าง	เครื่องมือตรวจวิเคราะห์
	ชื่อเครื่องมือ	ชื่อเครื่องมือ
คุณภาพอากาศในบรรยากาศ TSP	High Volume Air Sampler No. R05, R06, R07, R10	Digital Balance
PM ₁₀	High Volume PM10 Air Sampler No. R10, R12, R13, R14	Digital Balance
SO ₂	SO ₂ Analyzer No. R02, R04, R05, R06	SO2 Analyzer No. R02, R04, R05, R06
NO ₂	NO ₂ Analyzer No. B02, R04, R07, R08	NO Analyzer No. B02, R04, R07, R08
Acetaldehyde	Mass Flow Meter	GC/MS
คุณภาพอากาศจากปล่อง TSP	Console No. R04, R05 Pitot Tube No. B24, B33	Digital Balance
NO _x	Vacuum Gauge	Spectrophotometer
SO ₂	Personal Pump SKC No. R33 Rotameter No. H-R01, R02	-
Acetaldehyde	Personal Pump SKC No. R36 Rotameter No. H-R02	GC/FID
Ethylene Glycol	Personal Pump SKC No. B45 Rotameter No. H-R02	GC/FID
ระดับเสียง Leq 24 hr Lmax L90	Acoustic Calibrator	-
	Sound Level Meter No. ACO-R02, R48	
คุณภาพน้ำ pH	-	pH Meter
BOD ₅	-	DO Meter
COD	-	COD Reactor
Total Suspended Solids	-	Digital balances
Total Dissolved Solids	-	Digital balances
Grease and Oil	-	Digital balances
Ethylene Glycol	-	GC/FID
Acetaldehyde	-	GC/MS
Arsenic	-	AAS
Selenium	-	AAS
Mercury	-	AAS
Manganese	-	ICP

ตารางสรุปรายการเอกสารการสอบเทียบความถูกต้องของเครื่องมือเก็บตัวอย่างและตรวจวิเคราะห์ (ต่อ)

รายการตรวจวัด	เครื่องมือเก็บตัวอย่าง	เครื่องมือตรวจวิเคราะห์
	ชื่อเครื่องมือ	ชื่อเครื่องมือ
คุณภาพน้ำ (ต่อ) Zinc	-	ICP
Copper	-	ICP
Cadmium	-	ICP
Nickel	-	ICP
Lead	-	ICP
Barium	-	ICP
Trivalent Chromium	-	ICP Spectrophotometer
Hexavalent Chromium	-	Spectrophotometer
คุณภาพน้ำใต้ดิน Acetaldehyde	-	GC/MS
คุณภาพอากาศในสถานประกอบการ Acetaldehyde	Personal Pump No. B12, B61, B62, B72, B89, B93, R07, R25, R30, R34, R40 Rotameter No. L-R05, R06	GC/FID
Ethylene Glycol	Personal Pump No. B21, B61, B63, B72, B89, R07, R21, R25, R34, R40 Rotameter No. H-R05, R06	GC/FID
Total Dust	Personal Pump No. B12, B21, B45, B62, R11, R13, R26, R31 Rotameter No. H-R05, R06	Digital Balance
Respirable Dust	Personal Pump No. B21, B62, B70, B71, R13, R19, R31, R33 Rotameter No. H-R05, R06	Digital Balance
Phosphoric Acid	Personal Pump No. B45, B72, B76, R17, R37 Rotameter No. L-R05, R06	IC
Sodium Hydroxide	Personal Pump No. B12, B45, B63, R15, R39 Rotameter No. H-R05, R06	-
Sodium Hypochlorite as Sodium	Personal Pump No. B89, R28 Rotameter No. H-R05, R06	ICP
Hydrogen Sulfide	Personal Pump No B61, R40 Rotameter No. L-R05, R06	IC
Acetone	Personal Pump No. B89, R03 Rotameter No. L-R05, R06	GC/FID
Ethanol	Personal Pump No. B89, R03 Rotameter No. L-R05, R06	GC/FID
Chloroform	Personal Pump No. B63, R40 Rotameter No. L-R05, R06	GC/FID

ตารางสรุปรายการเอกสารการสอบเทียบความถูกต้องของเครื่องมือเก็บตัวอย่างและตรวจวิเคราะห์ (ต่อ)

รายการตรวจวัด	เครื่องมือเก็บตัวอย่าง	เครื่องมือตรวจวิเคราะห์
	ชื่อเครื่องมือ	ชื่อเครื่องมือ
คุณภาพอากาศในสถานประกอบการ (ต่อ) Phenol	Personal Pump No. B72, R21 Rotameter No. L-R05, R06	GC/FID
Isopropyl Alcohol	Personal Pump No. B81, R23 Rotameter No. L-R05, R06	GC/FID
Hydrochloric Acid	Personal Pump No. B71, R17 Rotameter No. L-R05, R06	IC
Acetic Acid	Personal Pump No. B12, B93, R10, R24 Rotameter No. L-R05, R06	GC/FID
ระดับเสียงในสถานประกอบการ Leq 12 hr Lmax	Acoustic Calibrator No. 130006	-
	Sound Level Meter No. ACO-R40, R41, R50, R51, R52	-
ปริมาณเสียงสะสมติดตัวพนักงาน Noise Dose	Acoustic Calibrator No. 83820	-
	Noise Dosimeter No. NMD-R02, R03, R06, R13, R22	-
ระดับความเข้มของแสงสว่างในสถาน ประกอบการ Light Intensity	Light Meter No. R07	-
ระดับความร้อนในสถานประกอบการ WBGT	Heat Stress WBGT Meter No. B21, B32, R05, R08	-

เอกสารแนบ 5-1

เอกสารสอบเทียบเครื่องมือการตรวจวัดคุณภาพอากาศในบรรยากาศ



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจตุจักร เขตจตุจักร กรุงเทพฯ 10900
Tel : (662) 939-4370-72 Fax : (662) 513-4221 E-mail : sales@spsc.com www.spsc.com

High Volume Air Sampler Calibration Report

Calibration Method : Multipoint Orifice Flow Transfer Standard Model : TE 5025A S/N : 3440

Calibration Data

High Volume Air Sampler Data		Calibration Data		
Recorder No.	Blower No.	Date	Actual Flowrate (ft ³ /min)	R ²
B01	B01	01/08/2025	$y = 1.099x - 3.517$	0.999
B02	B02	01/08/2025	$y = 1.142x - 3.995$	0.999
B03	B03	01/08/2025	$y = 1.127x - 5.756$	0.997
B04	B04	01/08/2025	$y = 1.137x - 4.695$	0.999
B05	B05	01/08/2025	$y = 1.128x - 5.472$	0.999
B06	B06	01/08/2025	$y = 1.177x - 5.925$	0.996
B07	B07	01/08/2025	$y = 1.147x - 5.407$	0.999
B08	B08	01/08/2025	$y = 1.152x - 6.011$	0.997
B09	B09	01/08/2025	$y = 1.132x - 4.325$	0.998
B10	B10	07/08/2025	$y = 1.123x - 5.255$	0.998
B11	B11	01/08/2025	$y = 1.131x - 3.867$	0.997
B12	B12	01/08/2025	$y = 1.128x - 2.501$	0.997
B13	B13	01/08/2025	$y = 1.162x - 4.037$	0.996
B14	B14	01/08/2025	$y = 1.144x - 4.295$	0.997
B15	B15	01/08/2025	$y = 1.101x - 3.061$	0.998
B16	B16	07/08/2025	$y = 1.039x - 1.195$	0.999
B17	B17	01/08/2025	$y = 1.056x + 0.573$	0.998
B18	B18	01/08/2025	$y = 1.176x - 6.349$	0.998
B19	B19	01/08/2025	$y = 1.150x - 4.805$	0.996
B20	B20	04/08/2025	$y = 1.043x + 2.427$	0.999
B21	B21	01/08/2025	$y = 1.064x + 0.460$	0.997
B22	B22	01/08/2025	$y = 1.146x - 4.084$	0.998
B23	B23	01/08/2025	$y = 1.118x - 2.441$	0.999
B24	B24	01/08/2025	$y = 1.085x - 1.292$	0.999
B25	B25	01/08/2025	$y = 1.074x + 0.323$	0.999
B26	B26	04/08/2025	$y = 1.098x - 3.782$	0.997
B27	B27	01/08/2025	$y = 1.173x - 7.561$	0.997
B28	B28	01/08/2025	$y = 1.128x - 5.410$	0.998
B29	B29	01/08/2025	$y = 1.134x - 3.750$	0.998
B30	B30	01/08/2025	$y = 1.050x + 1.266$	0.999
B31	B31	04/08/2025	$y = 1.166x - 5.291$	0.999
B32	B32	01/08/2025	$y = 1.159x - 4.739$	0.996
B33	B33	01/08/2025	$y = 1.173x - 5.447$	0.997
B34	B34	01/08/2025	$y = 1.148x - 4.099$	0.999

Calibrated by :

Adul Dangklom
(Mr. Adul Dangklom)

Approved by :

Peera Detudom
(Mr. Peera Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจตุจักร เขตจตุจักร กรุงเทพฯ 10900
Tel : (662) 939-4370-72 Fax : (662) 513-4221 E-mail : sales@spsc.com www.spsc.com

High Volume Air Sampler Calibration Report

Calibration Method : Multipoint Orifice Flow Transfer Standard Model : TE 5025A S/N : 3440

Calibration Data

High Volume Air Sampler Data		Calibration Data		
Recorder No.	Blower No.	Date	Actual Flowrate (ft ³ /min)	R ²
B35	B35	01/08/2025	$y = 1.126x - 2.314$	0.997
B36	B36	01/08/2025	$y = 1.158x - 3.625$	0.999
B37	B37	01/08/2025	$y = 1.071x - 0.714$	0.998
B38	B38	07/08/2025	$y = 1.138x - 6.470$	0.999
B39	B39	07/08/2025	$y = 1.074x - 2.233$	0.999
B40	B40	01/08/2025	$y = 1.137x - 4.281$	0.998
B41	B41	01/08/2025	$y = 1.124x - 3.061$	0.999
B42	B42	01/08/2025	$y = 1.130x - 3.831$	0.998
B43	B43	04/08/2025	$y = 1.098x - 1.647$	0.999
B44	B44	07/08/2025	$y = 1.107x - 2.029$	0.997
R01	R01	01/08/2025	$y = 1.027x + 1.685$	0.998
R02	R02	01/08/2025	$y = 1.154x - 5.444$	0.998
R03	R03	01/08/2025	$y = 1.174x - 5.934$	0.999
R04	R04	04/08/2025	$y = 1.125x - 3.465$	0.997
R05	R05	01/08/2025	$y = 1.097x + 0.437$	0.999
R06	R06	04/08/2025	$y = 1.138x - 2.560$	0.997
R07	R07	01/08/2025	$y = 1.046x - 0.699$	0.999
R08	R08	01/08/2025	$y = 1.109x - 3.582$	0.997
R09	R09	01/08/2025	$y = 1.088x - 1.852$	0.999
R10	R10	01/08/2025	$y = 1.134x - 4.535$	0.996
R11	R11	01/08/2025	$y = 1.170x - 6.929$	0.998
R12	R12	01/08/2025	$y = 1.151x - 4.183$	0.999
R13	R13	01/08/2025	$y = 1.117x - 4.198$	0.999
R14	R14	01/08/2025	$y = 1.109x - 2.662$	0.998
R15	R15	01/08/2025	$y = 1.126x - 5.806$	0.996
R16	R16	01/08/2025	$y = 1.149x - 7.086$	0.996
R17	R17	01/08/2025	$y = 1.120x - 5.050$	0.997
R18	R18	04/08/2025	$y = 1.155x - 5.737$	0.997
R19	R19	04/08/2025	$y = 1.131x - 5.715$	0.997
R20	R20	01/08/2025	$y = 1.152x - 5.912$	0.996

Calibrated by :

Adul Dangklom
(Mr. Adul Dangklom)

Approved by :

Peera Detudom
(Mr. Peera Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4231, E-mail : sale@spscon.com, www.spscon.com

High Volume PM-10 Air Sampler Calibration Report

Calibration Method : Multipoint Orifice Flow Transfer Standard Model : TE 5025A S/N : 3440

Calibration Data

High Volume PM-10 Data		Calibration Data		
Recorder No.	Blower No.	Date	Actual Flowrate (ft ³ /min)	R ²
B01	B01	01/08/2025	y = 1.114x-2.914	0.997
B02	B02	07/08/2025	y = 1.013x+1.223	0.998
B03	B03	01/08/2025	y = 1.161x-6.637	0.997
B04	B04	01/08/2025	y = 1.104x-4.741	0.999
B05	B05	01/08/2025	y = 1.139x-4.983	0.999
B06	B06	07/08/2025	y = 1.115x-4.334	0.997
B07	B07	01/08/2025	y = 1.134x-5.274	0.999
B08	B08	07/08/2025	y = 1.118x-2.369	0.999
B09	B09	01/08/2025	y = 1.043x-0.834	0.999
B10	B10	01/08/2025	y = 1.096x-2.892	0.998
B11	B11	01/08/2025	y = 1.114x-3.605	0.997
B12	B12	06/08/2025	y = 1.096x-2.892	0.998
B13	B13	04/08/2025	y = 1.112x-4.752	0.996
B14	B14	01/08/2025	y = 1.104x-3.418	0.997
B15	B15	01/08/2025	y = 1.119x-2.509	0.996
B16	B16	01/08/2025	y = 1.012x+1.776	0.996
B17	B17	04/08/2025	y = 1.094x-0.874	0.999
B18	B18	07/08/2025	y = 1.140x-5.779	0.997
B19	B19	04/08/2025	y = 1.087x-0.543	0.999
B20	B20	01/08/2025	y = 1.108x-3.582	0.997
B21	B21	01/08/2025	y = 1.138x-4.442	0.996
B22	B22	01/08/2025	y = 1.097x-3.833	0.999
B23	B23	01/08/2025	y = 1.127x-4.713	0.999
B24	B24	01/08/2025	y = 1.117x-4.019	0.999
B25	B25	01/08/2025	y = 1.137x-5.745	0.996
B26	B26	01/08/2025	y = 1.029x-0.023	0.998
B27	B27	01/08/2025	y = 1.136x-6.732	0.996
B28	B28	01/08/2025	y = 1.114x-4.531	0.999
B29	B29	01/08/2025	y = 1.126x-5.420	0.999
B30	B30	01/08/2025	y = 1.119x-4.736	0.998
B31	B31	01/08/2025	y = 1.011x+2.394	0.998
B32	B32	01/08/2025	y = 1.047x-0.534	0.999
B33	B33	01/08/2025	y = 1.052x-0.474	0.998
B34	B34	07/08/2025	y = 1.028x+2.008	0.997

Calibrated by :

Adul Dangklom
(Mr.Adul Dangklom)

Approved by :

Mr. Peera Detudom
(Mr. Peera Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4231, E-mail : sale@spscon.com, www.spscon.com

High Volume PM-10 Air Sampler Calibration Report

Calibration Method : Multipoint Orifice Flow Transfer Standard Model : TE 5025A S/N : 3440

Calibration Data

High Volume PM-10 Data		Calibration Data		
Recorder No.	Blower No.	Date	Actual Flowrate (ft ³ /min)	R ²
R01	R01	01/08/2025	y = 1.104x-5.304	0.998
R02	R02	01/08/2025	y = 1.064x-2.883	0.998
R03	R03	01/08/2025	y = 1.108x-4.353	0.999
R04	R04	01/08/2025	y = 1.101x-5.579	0.998
R05	R05	01/08/2025	y = 1.119x-5.074	0.996
R06	R06	04/08/2025	y = 1.127x-3.817	0.998
R07	R07	04/08/2025	y = 1.037x+1.136	0.998
R08	R08	01/08/2025	y = 1.042x+0.842	0.998
R09	R09	01/08/2025	y = 1.083x-2.007	0.997
R10	R10	01/08/2025	y = 1.041x-0.474	0.997
R11	R11	01/08/2025	y = 1.085x-1.404	0.997
R12	R12	01/08/2025	y = 1.062x-1.485	0.997
R13	R13	01/08/2025	y = 1.075x-2.468	0.999
R14	R14	01/08/2025	y = 1.017x+0.519	0.999
R15	R15	01/08/2025	y = 1.138x-6.436	0.998
R16	R16	04/08/2025	y = 1.051x+0.908	0.999
R17	R17	04/08/2025	y = 1.114x-4.329	0.998
R18	R18	01/08/2025	y = 1.098x-5.423	0.998
R19	R19	01/08/2025	y = 1.113x-2.373	0.997
R20	R20	01/08/2025	y = 1.105x-4.058	0.998

Calibrated by :

Adul Dangklom
(Mr.Adul Dangklom)

Approved by :

Mr. Peera Detudom
(Mr. Peera Detudom)



CERTIFICATE No : 25M2254
REFERENCE No : 76365-1

PAGE : 1 OF 2

Certificate of Calibration

EQUIPMENT : DIGITAL BALANCE
MANUFACTURER : METTLER TOLEDO
MODEL : XS105DU
SERIAL No : 1126422905
ID No : BA05/50
CONDITION AS RECEIVED : USED ITEM
SUBMITTED BY : S.P.S. CONSULTING SERVICE CO., LTD.
7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN RD.,
JOMPOL, CHATUCHAK, BANGKOK 10900

CALIBRATED BY : ATSAWIN Y.
CALIBRATION DATE : 07-Mar-25

APPROVED BY : PONGSAK J.
ISSUED DATE : 13-Mar-25
RECEIVED DATE : 07-Mar-25

THIS CERTIFICATE MAY NOT BE REPRODUCED OTHER THAN IN FULL EXCEPT WITH THE PRIOR WRITTEN APPROVAL OF
QUALITY CALIBRATION CO., LTD.



CERTIFICATE No : 25M2254

PAGE : 2 OF 2

Calibration Report

EQUIPMENT : DIGITAL BALANCE
MANUFACTURER : METTLER TOLEDO
ID No : BA05/50
AIR PRESSURE : 1009mbar \pm 1mbar
AMBIENT TEMPERATURE : 24°C \pm 1°C
MODEL : XS105DU
S/N : 1126422905
RECEIVED DATE : 07-Mar-25
CALIBRATION DATE : 07-Mar-25
RELATIVE HUMIDITY : 54%RH \pm 10% RH

CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED BY ACCORDING TO UKAS LAB 14 EDITION 6:2019 BY USING KNOWN WEIGHT STANDARD WEIGHT. THE BALANCE WAS NOT ADJUSTED BEFORE CALIBRATION. THE BALANCE HAS NO ZERO TRACKING FUNCTION. REPEATABILITY WAS MEASURED BY USING 10 REPEATED MEASUREMENTS. LINEARITY WAS MEASURED COVERING 10 POINTS, EVENLY SPREAD OVER THE RANGE. THE INSTRUMENT WAS SET ZERO BEFORE PERFORMING THE LINEARITY TEST. OFF-CENTER LOADING WAS MEASURED BY USING STANDARD WEIGHTS PLACED ON THE PAN AND MOVED TO VARIOUS POSITIONS ON THE PAN.

2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) STANDARD WEIGHT SET	E2	QK-I-151	C02250116	28-Jan-27
2) STANDARD WEIGHT	E2	15843	C02250117	29-Jan-27

3. THE CERTIFICATE IS VALID FOR THE ITEM CALIBRATED AS SHOWN ON THE DATE AND PLACE OF CALIBRATION ONLY.

4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.

5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-
- NATIONAL INSTITUTE OF METROLOGY (THAILAND)

RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

1. ZERO SETTING FUNCTION : NORMAL

2. TARE FUNCTION : NORMAL

3. REPEATABILITY OF READING AT 120 g WAS 0.000055 g

4. DEPARTURE FROM NOMINAL VALUE/ LINEARITY

NOMINAL VALUE (g)	BALANCE READING (g)	CORRECTION (g)	UNCERTAINTY (\pm g)
0.00	0.00000	0.00000	0.000065
0.02	0.01999	0.00001	0.000065
0.10	0.10001	-0.00001	0.000066
0.20	0.20001	-0.00001	0.000066
0.50	0.50002	-0.00002	0.000065
1.00	1.00003	-0.00003	0.000066
2.00	2.00001	-0.00001	0.000067
5.00	5.00002	-0.00002	0.000068
10.00	10.00000	0.00000	0.000070
20.00	20.00004	-0.00004	0.000078
50.00	50.00000	0.00000	0.00013
100.00	100.0001	-0.0001	0.00019
120.00	120.0002	-0.0002	0.00022

5. OFF CENTER LOADING ERROR



POINT	READING (g)
1	50.0000
2	50.0000
3	50.0000
4	50.0000
5	50.0000
OFF-CENTER LOADING	0.0000

NOTE: THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA
THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A
COVERAGE FACTOR $k=2$, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT





บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chaluchak, Bangkok 10900
Tel : (662) 939-9370-72, Fax : (662) 513-4221, E-mail : sales@spscon.com, www.spscon.com

CALIBRATION REPORT					
SO ₂ FLUORESCENT ANALYZER					
DATE :	19 August 2025	BRAND :	TELEDYNE	MODEL :	100E
NO.	SO ₂ -R02	SERIAL NO.	3431		
Calibrator (Dilution System)					
Brand : Teledyne		Model : 700			
Last Cal. Date : 29 October 2024		Serial No. : 421			
Reference Standard Gas					
Standard Gas : Sulphur Dioxide (SO ₂)		Cylinder No. : A008145K			
Certified Date : 21 June 2021		Expired Date : 21 June 2029		Cylinder Conc. : 49.8 ppm	
CALIBRATING CONDITION					
Pressure	1011	mmbar	Temp.	24.6	°C
% RH	49				
CALIBRATION SETTING					
Span	Initial Reading (Before Adj.),PPB			Final Reading (After Adj.),PPB	
Set Point	Expected Concentration	Analyzer Response	%Dif	Analyzer Response	Slope
Zero	0	0.10	-	0	-
SO ₂ Span	400.0	399.6	-0.100	400.0	1.006
API Model TML-60 SO ₂ Analyzer Check list					
Test Values	Observed Value	Units	Nominal Range		
RANGE	500	PPB	0-500		
SAMPLE PRESS	28.3	in-Hg	25-35		
SAMPLE FLOW	657	cc/min	650 ± 10%		
PMT	103.2	mV	-20-150 with Zero Air		
UV LAMP	3036.3	mV	1000-4900		
STR. LGT	61.8	PPB	<100		
DRK PMT	63.4	mV	-50 - 200		
DRK LMP	58.0	mV	-50 - 200		
HVPS	673	V	550-900 constant		
DCPS	2529	mV	2500 ± 200		
RCELL TEMP	50.3	°C	50 ± 1		
BOX TEMP	29.1	°C	5-40		
PMT TEMP	7.5	°C	7 ± 2.0		
SO ₂ Span Conc	400	PPB	20-20,000		
SO ₂ Slope	1.006	-	1.0 ± 0.3		
SO ₂ Offset	22.1	mV	<250		
Stability at Zero	0.1	PPB	<0.2		
Stability at Span	0.2	PPB	0.5% of reading (above 50 ppb)		

Calibrated by : Wu M
(Mr.Kaseam Simaphon)

Approved by : Yuthana J.
(Mr.Yuthana Thanataranit)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chaluchak, Bangkok 10900
Tel : (662) 939-9370-72, Fax : (662) 513-4221, E-mail : sales@spscon.com, www.spscon.com

CALIBRATION REPORT					
SO ₂ FLUORESCENT ANALYZER					
DATE :	19 August 2025	BRAND :	TELEDYNE	MODEL :	100E
NO.	SO ₂ -R04	SERIAL NO.	3489		
Calibrator (Dilution System)					
Brand : Teledyne		Model : 700			
Last Cal. Date : 29 October 2024		Serial No. : 421			
Reference Standard Gas					
Standard Gas : Sulphur Dioxide (SO ₂)		Cylinder No. : A008145K			
Certified Date : 21 June 2021		Expired Date : 21 June 2029		Cylinder Conc. : 49.8 ppm	
CALIBRATING CONDITION					
Pressure	1011	mmbar	Temp.	24.6	°C
% RH	49				
CALIBRATION SETTING					
Span	Initial Reading (Before Adj.),PPB			Final Reading (After Adj.),PPB	
Set Point	Expected Concentration	Analyzer Response	%Dif	Analyzer Response	Slope
Zero	0	0.11	-	0	-
SO ₂ Span	400.0	400.1	0.025	400.0	1.012
API Model TML-60 SO ₂ Analyzer Check list					
Test Values	Observed Value	Units	Nominal Range		
RANGE	500	PPB	0-500		
SAMPLE PRESS	28.7	in-Hg	25-35		
SAMPLE FLOW	653	cc/min	650 ± 10%		
PMT	103.0	mV	-20-150 with Zero Air		
UV LAMP	3021.8	mV	1000-4900		
STR. LGT	61.5	PPB	<100		
DRK PMT	62.9	mV	-50 - 200		
DRK LMP	57.6	mV	-50 - 200		
HVPS	669	V	550-900 constant		
DCPS	2520	mV	2500 ± 200		
RCELL TEMP	50.4	°C	50 ± 1		
BOX TEMP	29.3	°C	5-40		
PMT TEMP	7.2	°C	7 ± 2.0		
SO ₂ Span Conc	400	PPB	20-20,000		
SO ₂ Slope	1.012	-	1.0 ± 0.3		
SO ₂ Offset	21.8	mV	<250		
Stability at Zero	0.1	PPB	<0.2		
Stability at Span	0.2	PPB	0.5% of reading (above 50 ppb)		

Calibrated by : Wu A
(Mr.Kaseam Simaphon)


Approved by : Yuthana J.
(Mr.Yuthana Thanataranit)




บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจตุจักร เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chaluchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spicon.com, www.spicon.com

CALIBRATION REPORT					
SO ₂ FLUORESCENT ANALYZER					
DATE :	19 August 2025	BRAND :	API	MODEL :	100E
NO.	SO ₂ -R05	SERIAL NO.	3490		
Calibrator (Dilution System)					
Brand	: Teledyne		Model	: 700	
Last Cal. Date	: 29 October 2024		Serial No.	: 421	
Reference Standard Gas					
Standard Gas	: Sulphur Dioxide (SO ₂)		Cylinder No.	: A00814SK	
Certified Date	: 21 June 2021		Expired Date	: 21 June 2029	
			Cylinder Conc.	: 49.8 ppm	
CALIBRATING CONDITION					
Pressure	1011	mmbar	Temp.	24.6	°C
			% RH	49	
CALIBRATION SETTING					
Span	Initial Reading (Before Adj.),PPB			Final Reading (After Adj.),PPB	
Set Point	Expected Concentration	Analyzer Response	%Dif	Analyzer Response	Slope
Zero	0	0.10	-	0	-
SO ₂ Span	400.0	399.8	-0.050	400.0	1.007
API Model 100E SO ₂ Analyzer Check list					
Test Values	Observed Value	Units	Nominal Range		
RANGE	500	PPB	0-500		
SAMPLE PRESS	28.3	in-Hg	25-35		
SAMPLE FLOW	660	cc/min	650 ± 10%		
PMT	103.2	mV	-20-150 with Zero Air		
UV LAMP	3038.6	mV	1000-4900		
STR. LGT	61.5	PPB	<100		
DRK PMT	63.0	mV	-50 - 200		
DRK LMP	57.7	mV	-50 - 200		
HVPS	671	V	550-900 constant		
DCPS	2526	mV	2500 ± 200		
RCCELL TEMP	50.0	°C	50 ± 1		
BOX TEMP	29.3	°C	5-40		
PMT TEMP	7.1	°C	7 ± 2.0		
SO ₂ Span Conc	400	PPB	20-20,000		
SO ₂ Slope	1.007	-	1.0 ± 0.3		
SO ₂ Offset	21.6	mV	<250		
Stability at Zero	0.1	PPB	<0.2		
Stability at Span	0.2	PPB	0.5% of reading (above 50 ppb)		

Calibrated by :


(Mr.Kaseam Simaphon)

Approved by :


(Mr.Yuthana Thanataranit)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจตุจักร เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chaluchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spicon.com, www.spicon.com

CALIBRATION REPORT					
SO ₂ FLUORESCENT ANALYZER					
DATE :	19 August 2025	BRAND :	API	MODEL :	100E
NO.	SO ₂ -R06	SERIAL NO.	066		
Calibrator (Dilution System)					
Brand	: Teledyne		Model	: 700	
Last Cal. Date	: 29 October 2024		Serial No.	: 421	
Reference Standard Gas					
Standard Gas	: Sulphur Dioxide (SO ₂)		Cylinder No.	: A00814SK	
Certified Date	: 21 June 2021		Expired Date	: 21 June 2029	
			Cylinder Conc.	: 49.8 ppm	
CALIBRATING CONDITION					
Pressure	1011	mmbar	Temp.	24.6	°C
			% RH	49	
CALIBRATION SETTING					
Span	Initial Reading (Before Adj.),PPB			Final Reading (After Adj.),PPB	
Set Point	Expected Concentration	Analyzer Response	%Dif	Analyzer Response	Slope
Zero	0	0.10	-	0	-
SO ₂ Span	400.0	399.7	-0.075	400.0	1.008
API Model 100E SO ₂ Analyzer Check list					
Test Values	Observed Value	Units	Nominal Range		
RANGE	500	PPB	0-500		
SAMPLE PRESS	28.4	in-Hg	25-35		
SAMPLE FLOW	654	cc/min	650 ± 10%		
PMT	103.5	mV	-20-150 with Zero Air		
UV LAMP	3054.2	mV	1000-4900		
STR. LGT	61.9	PPB	<100		
DRK PMT	63.5	mV	-50 - 200		
DRK LMP	58.1	mV	-50 - 200		
HVPS	670	V	550-900 constant		
DCPS	2517	mV	2500 ± 200		
RCCELL TEMP	50.2	°C	50 ± 1		
BOX TEMP	29.0	°C	5-40		
PMT TEMP	7.1	°C	7 ± 2.0		
SO ₂ Span Conc	400	PPB	20-20,000		
SO ₂ Slope	1.008	-	1.0 ± 0.3		
SO ₂ Offset	21.6	mV	<250		
Stability at Zero	0.1	PPB	<0.2		
Stability at Span	0.2	PPB	0.5% of reading (above 50 ppb)		

Calibrated by :


(Mr.Kaseam Simaphon)

Approved by :


(Mr.Yuthana Thanataranit)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chaluchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

CALIBRATION REPORT					
CHEMILUMINESCENT NO / NO ₂ / NO _x ANALYZER					
DATE :	19 August 2025	BRAND :	API	MODEL :	200A
NO.	NOX-B02	SERIAL NO.	2409		
Calibrator (Dilution System)					
Brand	: Teledyne		Model	: 700	
Last Cal. Date	: 29 October 2024		Serial No.	: 421	
Reference Standard Gas					
Standard Gas	: Nitric Oxide (NO)		Cylinder No.	: A00726SV	
Certified Date	: 05 January 2023		Expired Date	: 05 January 2026	
Cylinder Conc.	: 48.8 ppm				
CALIBRATING CONDITION					
Pressure	1011	mmbar	Temp.	24.6	°C
% RH	50				
CALIBRATION SETTING					
Span	Initial Reading (Before Adj.),PPB			Final Reading (After Adj.),PPB	
Set Point	Expected Concentration	Analyzer Response	%Dif	Analyzer Response	Slope
Zero	0	0.11	-	0	-
NO Span	400	400.1	0.025	400.0	1.010
NO _x Span	400	400.3	0.075	400.0	1.014
API Model 200A NO _x Analyzer Check List					
Test Values	Observed Value	Units	Nominal Range		
RANGE	500	PPB	500 standard		
STABILITY (Zero Gas)	0.1	PPB	< 2 with zero air		
SAMPLE FLOW	507	cc/min	500 ± 50		
OZONE FLOW	78	cc/min	80 ± 15		
PMT	103.1	mV	-20 - 150		
AZERO	93.9	mV	-20 - 150		
HVPS	674	V	420 - 900 constant		
RCCELL TEMP	50.0	°C	50 ± 1		
BOX TEMP	28.8	°C	8 - 48		
PMT TEMP	7.1	°C	7 ± 2		
MOLY TEMP	315.2	°C	315 ± 5		
RCCELL PRESS	8.3	IN-Hg-A	2 - 10 constant		
SAMPLE PRESS	28.5	IN-Hg-A	25 - 30 constant		
NO Span Conc	400	PPB	20 - 20,000		
NO _x Span Conc	400	PPB	20 - 20,000		
NO Slope	1.010	-	1.0 ± 0.3		
NO _x Slope	1.014	-	1.0 ± 0.3		
NO Offset	1.7	mV	-20 to +150		
NO _x Offset	1.0	mV	-20 to 150		
Stability at Zero	0.1	PPB	< 0.2		
Stability at Span	0.2	PPB	< 2 ppb @ 400 ppb span gas		

Calibrated by :

(Mr.Kasearn Simaphon)

Approved by :

(Mr.Yuthana Thanataranit)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chaluchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

CALIBRATION REPORT					
CHEMILUMINESCENT NO / NO ₂ / NO _x ANALYZER					
DATE :	19 August 2025	BRAND :	API	MODEL :	200E
NO.	NOX-R04	SERIAL NO.	4411		
Calibrator (Dilution System)					
Brand	: Teledyne		Model	: 700	
Last Cal. Date	: 29 October 2024		Serial No.	: 421	
Reference Standard Gas					
Standard Gas	: Nitric Oxide (NO)		Cylinder No.	: A00726SV	
Certified Date	: 05 January 2023		Expired Date	: 05 January 2026	
Cylinder Conc.	: 48.8 ppm				
CALIBRATING CONDITION					
Pressure	1011	mmbar	Temp.	24.6	°C
% RH	50				
CALIBRATION SETTING					
Span	Initial Reading (Before Adj.),PPB			Final Reading (After Adj.),PPB	
Set Point	Expected Concentration	Analyzer Response	%Dif	Analyzer Response	Slope
Zero	0	0.10	-	0	-
NO Span	400	400.1	0.025	400.0	1.008
NO _x Span	400	400.2	0.050	400.0	1.011
API Model 200E NO _x Analyzer Check List					
Test Values	Observed Value	Units	Nominal Range		
RANGE	500	PPB	500 standard		
STABILITY (Zero Gas)	0.1	PPB	< 2 with zero air		
SAMPLE FLOW	505	cc/min	500 ± 50		
OZONE FLOW	78	cc/min	80 ± 15		
PMT	103.2	mV	-20 - 150		
AZERO	93.9	mV	-20 - 150		
HVPS	670	V	420 - 900 constant		
RCCELL TEMP	50.2	°C	50 ± 1		
BOX TEMP	29.0	°C	8 - 48		
PMT TEMP	7.1	°C	7 ± 2		
MOLY TEMP	315.3	°C	315 ± 5		
RCCELL PRESS	8.4	IN-Hg-A	2 - 10 constant		
SAMPLE PRESS	28.6	IN-Hg-A	25 - 30 constant		
NO Span Conc	400	PPB	20 - 20,000		
NO _x Span Conc	400	PPB	20 - 20,000		
NO Slope	1.008	-	1.0 ± 0.3		
NO _x Slope	1.011	-	1.0 ± 0.3		
NO Offset	1.6	mV	-20 to +150		
NO _x Offset	1.0	mV	-20 to 150		
Stability at Zero	0.1	PPB	< 0.2		
Stability at Span	0.2	PPB	< 2 ppb @ 400 ppb span gas		

Calibrated by :

(Mr.Kasearn Simaphon)

Approved by :

(Mr.Yuthana Thanataranit)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจตุจักร เขตจตุจักร กรุงเทพฯ 10900
/ Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chulachak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com




บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจตุจักร เขตจตุจักร กรุงเทพฯ 10900
/ Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chulachak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

CALIBRATION REPORT					
CHEMILUMINESCENT NO / NO ₂ / NO _x ANALYZER					
DATE :	19 August 2025	BRAND :	API	MODEL :	200E
NO.	NOX-R07	SERIAL NO.	4468		
Calibrator (Dilution System)					
Brand	: Teledyne		Model	: 700	
Last Cal. Date	: 29 October 2024		Serial No.	: 421	
Reference Standard Gas					
Standard Gas	: Nitric Oxide (NO)		Cylinder No.	: A007265V	
Certified Date	: 05 January 2023	Expired Date	: 05 January 2026	Cylinder Conc.	: 48.8 ppm
CALIBRATING CONDITION					
Pressure	1011	mmbar	Temp.	24.6	°C
			% RH	48	
CALIBRATION SETTING					
Span	Initial Reading (Before Adj.),PPB			Final Reading (After Adj.),PPB	
Set Point	Expected Concentration	Analyzer Response	%Dif	Analyzer Response	Slope
Zero	0	-0.10	-	0	-
NO Span	400	400.1	0.025	400.0	1.009
NO _x Span	400	400.2	0.050	400.0	1.012
API Model 200E NO _x Analyzer Check List					
Test Values	Observed Value	Units	Nominal Range		
RANGE	500	PPB	500 standard		
STABILITY (Zero Gas)	0.1	PPB	< 2 with zero air		
SAMPLE FLOW	506	cc/min	500 ± 50		
OZONE FLOW	78	cc/min	80 ± 15		
PMT	103.2	mV	-20 - 150		
AZERO	94.0	mV	-20 - 150		
HVPS	672	V	420 - 900 constant		
RCELL TEMP	50.1	°C	50 ± 1		
BOX TEMP	29.3	°C	8 - 48		
PMT TEMP	7.2	°C	7 ± 2		
MOLY TEMP	314.7	°C	315 ± 5		
RCELL PRESS	8.4	IN-Hg-A	2 - 10 constant		
SAMPLE PRESS	28.7	IN-Hg-A	25 - 30 constant		
NO Span Conc	400	PPB	20 - 20,000		
NO _x Span Conc	400	PPB	20 - 20,000		
NO Slope	1.009	-	1.0 ± 0.3		
NO _x Slope	1.012	-	1.0 ± 0.3		
NO Offset	1.7	mV	-20 to +150		
NO _x Offset	1.0	mV	-20 to 150		
Stability at Zero	0.1	PPB	< 0.2		
Stability at Span	0.2	PPB	< 2 ppb @ 400 ppb span gas		


Calibrated by :


(Mr.Kaseam Simaphon)

Approved by :


(Mr.Yuthana Thanataranit)

Calibrated by :


(Mr.Kaseam Simaphon)

Approved by :


(Mr.Yuthana Thanataranit)

CALIBRATION REPORT					
CHEMILUMINESCENT NO / NO ₂ / NO _x ANALYZER					
DATE :	19 August 2025	BRAND :	API	MODEL :	200E
NO.	NOX-R08	SERIAL NO.	243		
Calibrator (Dilution System)					
Brand	: Teledyne		Model	: 700	
Last Cal. Date	: 29 October 2024		Serial No.	: 421	
Reference Standard Gas					
Standard Gas	: Nitric Oxide (NO)		Cylinder No.	: A007265V	
Certified Date	: 05 January 2023	Expired Date	: 05 January 2026	Cylinder Conc.	: 48.8 ppm
CALIBRATING CONDITION					
Pressure	1011	mmbar	Temp.	24.6	°C
			% RH	50	
CALIBRATION SETTING					
Span	Initial Reading (Before Adj.),PPB			Final Reading (After Adj.),PPB	
Set Point	Expected Concentration	Analyzer Response	%Dif	Analyzer Response	Slope
Zero	0	-0.10	-	0	-
NO Span	400	400.1	0.025	400.0	1.009
NO _x Span	400	400.3	0.075	400.0	1.013
API Model 200E NO _x Analyzer Check List					
Test Values	Observed Value	Units	Nominal Range		
RANGE	500	PPB	500 standard		
STABILITY (Zero Gas)	0.1	PPB	< 2 with zero air		
SAMPLE FLOW	513	cc/min	500 ± 50		
OZONE FLOW	79	cc/min	80 ± 15		
PMT	103.5	mV	-20 - 150		
AZERO	94.2	mV	-20 - 150		
HVPS	672	V	420 - 900 constant		
RCELL TEMP	50.1	°C	50 ± 1		
BOX TEMP	29.4	°C	8 - 48		
PMT TEMP	7.2	°C	7 ± 2		
MOLY TEMP	315.2	°C	315 ± 5		
RCELL PRESS	8.4	IN-Hg-A	2 - 10 constant		
SAMPLE PRESS	28.6	IN-Hg-A	25 - 30 constant		
NO Span Conc	400	PPB	20 - 20,000		
NO _x Span Conc	400	PPB	20 - 20,000		
NO Slope	1.009	-	1.0 ± 0.3		
NO _x Slope	1.013	-	1.0 ± 0.3		
NO Offset	1.6	mV	-20 to +150		
NO _x Offset	1.1	mV	-20 to 150		
Stability at Zero	0.1	PPB	< 0.2		
Stability at Span	0.2	PPB	< 2 ppb @ 400 ppb span gas		



MIRACLE INTERNATIONAL TECHNOLOGY CO.,LTD

214 Bangwaek Rd. Bangpai Bangkok 10160
Tel.: 0-2865-4647-8 Fax: 0-2865-4649 http://www.mit.in.th



CALIBRATION CERTIFICATE

Page 1 of 4

Certificate No. : L202412119-0001

Date Issued : 13-Dec-24

Customer : S.P.S. CONSULTING SERVICE CO., LTD.
7 Soi Phaholyothin 24 Phaholyothin Road., Jompol, Chatuchak,
Bangkok 10900

Equipment : Mass Flow meter

Manufacturer : Dwyer

Model : GMF-2101

Serial No. : -

ID No./Tag No. : MF01/51

Date Received : 11-Dec-24

Date Calibrated : 12-Dec-24

Calibrated by : Saruth Srichutikul

Calibration Method or Calibration Procedure Used

In-house method : CP-34 by comparison against mass flow calibrator.

This certificate is traceable to national standards, which realize the units of measurement according to the International System of Units (SI).

Result of Calibration

The reported uncertainty of measurement was based on standard uncertainty multiplied by a coverage factor $k = 2$, providing a level confidence approximately 95 percent.

This certificate may not be reproduced other than in full except with the prior written approval of the Miracle International Technology Company Limited.

Approved by:

Sarayuth T.
(Sarayuth Tochua)



Certificate No. : L202412119-0001

Ambient Temperature : $(25 \pm 2)^\circ\text{C}$

Relative Humidity : $(50 \pm 15)\%\text{RH}$

Capacity Range : 17 ml/min

Calibration Media : Air


Type : Mass Flowmeter

Unit Under Calibration Reference Condition : Pressure 101.325 kPa(abs) , 21°C , Nitrogen

Before Adjustment

Temperature ($^\circ\text{C}$)	Pressure (kPa)	UUC Reading (ml/min)	STD Reading (ml/min)	Error (ml/min)	Uncertainty (\pm ml/min)
24.00	100.46	0.00	0.000 *	0.000	0.063
24.10	100.62	3.30	3.149	0.151	0.13
24.10	100.78	7.30	7.2	0.10	0.14
24.20	101.07	13.50	13.7	-0.20	0.15
24.20	101.30	17.00	18.3	-1.30	0.19

Error = Unit Under Calibration - Standard

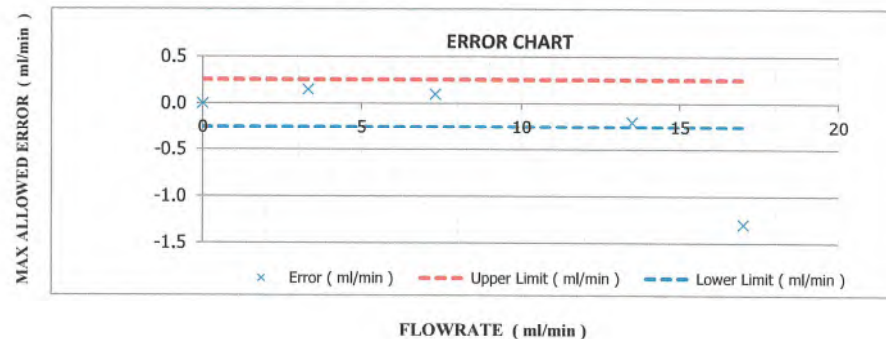

Certificate No. : L202412119-0001

Ambient Temperature : (25 ± 2)°C

Relative Humidity : (50 ± 15)%RH

Capacity Range : 17 ml/min

Calibration Media : Air


Type : Mass Flowmeter

Unit Under Calibration Reference Condition : Pressure 101.325 kPa(abs) , 21 °C , Nitrogen

After Adjustment

Temperature (° C)	Pressure (kPa)	UUC Reading (ml/min)	STD Reading (ml/min)	Error (ml/min)	Uncertainty (± ml/min)
24.00	100.45	0.00	0.000 *	0.000	0.063
24.10	100.62	3.30	3.170	0.130	0.13
24.10	100.78	7.30	7.2	0.10	0.14
24.20	101.01	13.50	13.6	-0.10	0.15
24.00	101.19	17.00	17.1	-0.10	0.18

Error = Unit Under Calibration - Standard

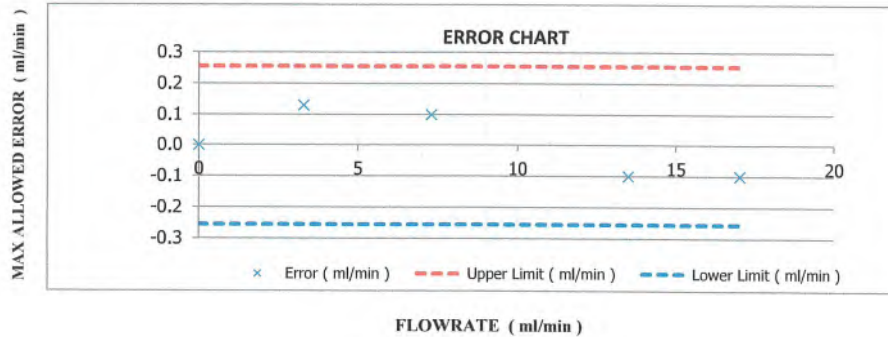

Certificate No. : L202412119-0001

Note : The actual flow rate is determined by the equation :

$$Q_{Meas} = Q_{Ref} \times \frac{P_{Ref}}{P_{Meas}} \times \frac{T_{Meas}}{T_{Ref}}$$

; Q = Flow rate

; P = Absolute pressure

; T = Absolute temperature

; Subscript "Meas" = Measurement condition

; Subscript "Ref" = Reference condition

Condition As-Received : Used Item

The measurement results and statements of conformity with specification only relate to the item calibrated.

Traceability of Certificate :


The International System of Units (SI) through

NIMT Certificate No. MW-0047-24, MW-0048-24 for Gas Flow meter Serial No. M5209179B/M5209179A, Due 03-Jul-25

End of Certificate

GC Clarus 600/680 Preventive Maintenance (PM)

Company Name:	S.P.S. Consulting Service Co.,Ltd		
Address (Instrument Location):	7 Soi Phaholyothin24 Phaholyothin Road, Jompol, Chatuchak, Bangkok, 10900.		
Serial Number:	680S14042502	Service Tag:	N68APSSFEMP
Customer Name (if applicable):	Ms.Naruecha	PM number :	2 of 2
Service Engineer Name:	Monchai Kitcharoenkeat	Service Order Number:	WO-06815714
Date PM Performed: (DD-MMM-YYYY)	13-Aug-2025	Next PM Due Date: (DD-MMM-YYYY)	13-Feb-2026

Part Number	Release	Publication Date	
TH09370070	C	August 2016	

Scope

The purpose of this PM is to ensure the continued functionality of the Clarus 600 and Clarus 680 GC by inspecting and replacing any worn or damaged parts. This service should only be performed by a trained representative of PerkinElmer. The customer should save their method before the PM begins.

General Instructions:

The customer must provide the engineer operational data to demonstrate recent instrument performance prior to starting the PM. Always check with the customer before making any changes that may affect the customer's analysis or calibration, including a current back-up of system software and/or data files. The completed document should be signed by an authorized PerkinElmer and customer representative and left with the customer. Update the PM sticker and instrument logbook as required.

Copyright Information

This document contains proprietary information that is protected by copyright. All rights are reserved. No part of this publication may be reproduced in any form whatsoever or translated into any language without the prior, written permission of Perkin Elmer, Inc. Copyright © 2013 PerkinElmer, Inc.

Trademarks

Registered names, trademarks, etc. used in this document, even when not specifically marked as such, are protected by law. PerkinElmer is a registered trademark of PerkinElmer, Inc. All other trademarks and registered trademarks not owned by PerkinElmer, Inc. or its subsidiaries that are depicted herein are the property of their respective owners. **Except as specifically set forth in its terms and conditions of sale, PerkinElmer makes no Warranty of any kind with regard to this document, including, but not limited to, the implied warranties of merchantability and fitness for a particular purpose.** PerkinElmer shall not be liable for incidental or consequential damages in connection with the furnishing or use of this document.

Component List

Component / Specific Model	Serial #	Software Version	Configuration Notes
Clarus680	680S14042502	Totalchrom6.3.2	PSS, PSS, FID,
Clarus SQ8T	648N4050804	Turbomass 6.4	
AtomX	US14113002	Tekma AtomX	

Parts Lists

Additional Tools Required for PM				
Part Number (if applicable)	Description	Quantity	Serial #	Calibration Due Date (MM/YY)
N/A				
Additional Reagents and Standards Required for PM				
Part Number (if applicable)	Description	Quantity	Batch/Lot #	Expiration Date (MM/YY)
N/A				

Procedure Checklist

Use (✓) to check off those steps in the checklist that have been completed.

1. General:

- ☒ Review the instrument performance with the customer and document any recent problems.
- ☒ Check incoming AC line voltage for proper levels and grounding.
 L-N 220 Volt
 L-G 220 Volt
 N-G 0.32 Volt

**Neutral to ground not more than 0.5 volts peak to peak*
- ☒ Inspect all gas line filters and traps; Replace if necessary with customer supplied spares.
 Carrier gas ☒ Helium ☐ Nitrogen ☐ Hydrogen
 Moisture level ☒ Good ☐ Need to replace ☐ Other _____

 Detector gas ☒ Air Zero ☒ Hydrogen ☐ Nitrogen ☐ Helium
 Moisture level ☒ Good ☐ Need to replace ☐ Other _____
- ☒ Inspect the customer log book and make any appropriate PM entries.
- ☒ Leak check all fittings from the gas source to instrument.
 Gas leakage ☒ Pass ☐ Fail Comment _____
- ☒ Perform general inspection of system for cleanliness.
- ☒ Inspect for functional and clean electronic cooling and oven vent fans
 Electronic cooling fan ☒ Yes ☐ No
 Oven cooling fan ☒ Yes ☐ No

2. Electronic :

- ☒ Check oven temperature. Calibrate if necessary.
 Oven temperature set point 150 °C ☒ Pass ☐ Fail
- ☐ Check sub-ambient option. (If installed).
 Oven temperature set point 5 °C ☐ Pass ☐ Fail
- ☒ Perform routine maintenance on detector/injector. Replace parts as necessary with customer supplied spares.

- ☒ Check flows, including split flows if applicable. Calibrate if necessary.
 Carrier flow ☒ Pass
 Split flow ☒ Pass
- ☒ Check detector gas flows and adjust if necessary.
 Detector flow ☒ Pass
- ☒ Autosampler installed ☒ Yes ☐ No
 Check autosampler sensor for wear and replace if necessary.
 Vial sensor ☒ Pass
 Door sensor ☒ Pass
 Tower sensor ☒ Pass
 Plunger sensor ☒ Pass
 Elevator sensor ☒ Pass
- ☒ Remove syringe, manually flush. Replace with customer supplied spare if necessary.
- ☒ Check firmware version. Upgrade to current levels if necessary.
 Firmware version 6.5
- ☒ Measure all accessible power supply voltages.
 5 Volt ☒ Pass
 +15 Volt ☒ Pass
 -15 Volt ☒ Pass
 24 Volt ☒ Pass
- ☒ Record all detector voltage signal.
 Detector Channel A 0.98 mV.
 Detector Channel B NA mV.

3. Diagnostics Tests:

- ☒ Run instrument diagnostics.
 BRAM ☒ Pass
 EPROM ☒ Pass
- ☒ Run Autosampler diagnostics.
 BRAM ☒ Pass
 EPROM ☒ Pass

4. Review:

- ☒ Review with the customer PM work performed.
- ☒ Review with the customer routine maintenance procedures.
- ☒ Discuss recommended customer-supplied materials to have on hand
- ☒ Attach PM sticker.
- ☒ Update Logbook.

Additional Comments

Additional Comments Regarding the PM

Review

<i>The preventive maintenance checks and if applicable performance tests for Clarus600/680 GC have been completed.</i>	
<i>This Clarus600/680 GC Pass the preventive maintenance.</i>	
Review of Preventive Maintenance:	
Authorized PerkinElmer Representative: Monchai Kitcharoenkeat <i>Monchai</i>	Date: 13-Aug-2025 (DD-MMM-YYYY)
Authorized Customer Representative: Ms.Naruecha <i>Naruecha</i>	Date: 13-Aug-2025 (DD-MMM-YYYY)

เอกสารแนบ 5-2

เอกสารสอบเทียบเครื่องมือการตรวจวัดคุณภาพอากาศจากปล่อง



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด

S.P.S. CONSULTING SERVICE CO., LTD.

7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900

7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900

Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com., www.spscon.com

Console Calibration Report

Calibration Method

Critical Orifices

Calibration Data

Console Data		Calibration Data		
No.	Serial No.	Date	y	DH _g (mmH ₂ O)
B01	1563	02/06/2025	0.997	49.56
B02	8002514	04/06/2025	0.998	49.74
B03	1503016	02/06/2025	1.007	49.69
B04	00006659	04/06/2025	0.999	50.11
B05	00007428	02/06/2025	1.006	49.65
R01	1561	04/06/2025	1.003	49.70
R02	8002513	03/06/2025	0.998	49.82
R03	1570	03/06/2025	1.005	49.88
R04	8002519	02/06/2025	1.004	49.76
R05	1503015	04/06/2025	0.997	50.04

Remark : Accept Value of y (test) is $0.97 < y < 1.03$

Accept Value of DH_g (test) is 46.7 ± 6.4 (mmH₂O)

Calibrated by :

Adul Dangklom

(Mr. Adul Dangklom)

Approved by :

Peera Detudom

(Mr. Peera Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจตุจักร กรุงเทพมหานคร 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72 Fax : (662) 513-4221 E-mail : sale@spscon.com, www.spscon.com

Pitot Tube Calibration Report

Calibration Method

Standard Pitot Tube

Calibration Data

Pitot Tube Data			Calibration Data		
No.	Type of Pitot	Coefficient of Standard Pitot	Date	Avg. of Cp (test)	
				Side A	Side B
B03	S	0.99	04/08/2025	0.84	0.84
B04	S	0.99	01/08/2025	0.84	0.83
B05	S	0.99	01/08/2025	0.84	0.84
B07	S	0.99	04/08/2025	0.85	0.84
B08	S	0.99	01/08/2025	0.84	0.84
B09	S	0.99	04/08/2025	0.84	0.83
B11	S	0.99	05/08/2025	0.84	0.84
B16	S	0.99	04/08/2025	0.84	0.83
B18	S	0.99	01/08/2025	0.84	0.84
B19	S	0.99	01/08/2025	0.84	0.83
B21	S	0.99	04/08/2025	0.84	0.83
B24	S	0.99	01/08/2025	0.84	0.84
B27	S	0.99	04/08/2025	0.84	0.83
B30	S	0.99	01/08/2025	0.85	0.84
B31	S	0.99	01/08/2025	0.84	0.85
B33	S	0.99	01/08/2025	0.83	0.84
B35	S	0.99	01/08/2025	0.84	0.85

Remark : Accept value of Cp (test) is 0.84 ± 0.01

Calibrated by :

Adul Dangklom
(Mr. Adul Dangklom)

Approved by :

Peera Detudom
(Mr. Peera Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจตุจักร กรุงเทพมหานคร 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72 Fax : (662) 513-4221 E-mail : sale@spscon.com, www.spscon.com

Pitot Tube Calibration Report

Calibration Method

Standard Pitot Tube

Calibration Data

Pitot Tube Data			Calibration Data		
No.	Type of Pitot	Coefficient of Standard Pitot	Date	Avg. of Cp (test)	
				Side A	Side B
B36	S	0.99	01/08/2025	0.84	0.84
B37	S	0.99	01/08/2025	0.84	0.85
B38	S	0.99	01/08/2025	0.84	0.83
B39	S	0.99	01/08/2025	0.84	0.84
B40	S	0.99	04/08/2025	0.85	0.84
B41	S	0.99	01/08/2025	0.84	0.84
B44	S	0.99	05/08/2025	0.83	0.84
B45	S	0.99	01/08/2025	0.84	0.85
B46	S	0.99	01/08/2025	0.85	0.84
B47	S	0.99	01/08/2025	0.85	0.84
B48	S	0.99	01/08/2025	0.84	0.84
B49	S	0.99	04/08/2025	0.85	0.84
B54	S	0.99	01/08/2025	0.84	0.84
B56	S	0.99	04/08/2025	0.84	0.84
B57	S	0.99	04/08/2025	0.85	0.84
B58	S	0.99	04/08/2025	0.84	0.84

Remark : Accept value of Cp (test) is 0.84 ± 0.01

Calibrated by :

Adul Dangklom
(Mr. Adul Dangklom)

Approved by :

Peera Detudom
(Mr. Peera Detudom)



CERTIFICATE No : 25M2254
REFERENCE No : 76365-1

PAGE : 1 OF 2

Certificate of Calibration

EQUIPMENT : DIGITAL BALANCE
MANUFACTURER : METTLER TOLEDO
MODEL : XS105DU
SERIAL No : 1126422905
ID No : BA05/50
CONDITION AS RECEIVED : USED ITEM
SUBMITTED BY : S.P.S. CONSULTING SERVICE CO., LTD.
7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN RD.,
JOMPOL, CHATUCHAK, BANGKOK 10900

CALIBRATED BY : ATSAWIN Y.
CALIBRATION DATE : 07-Mar-25

APPROVED BY : PONGSAK J.
ISSUED DATE : 13-Mar-25
RECEIVED DATE : 07-Mar-25

THIS CERTIFICATE MAY NOT BE REPRODUCED OTHER THAN IN FULL EXCEPT WITH THE PRIOR WRITTEN APPROVAL OF
QUALITY CALIBRATION CO., LTD.



CERTIFICATE No : 25M2254

PAGE : 2 OF 2

Calibration Report

EQUIPMENT : DIGITAL BALANCE MODEL : XS105DU
MANUFACTURER : METTLER TOLEDO S/N : 1126422905
ID No : BA05/50 RECEIVED DATE : 07-Mar-25
AIR PRESSURE : 1009mbar \pm 1mbar CALIBRATION DATE : 07-Mar-25
AMBIENT TEMPERATURE : 24°C \pm 1°C RELATIVE HUMIDITY : 54%RH \pm 10% RH

CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED BY ACCORDING TO UKAS LAB 14 EDITION 6:2019 BY USING KNOWN WEIGHT STANDARD WEIGHT. THE BALANCE WAS NOT ADJUSTED BEFORE CALIBRATION. THE BALANCE HAS NO ZERO TRACKING FUNCTION. REPEATABILITY WAS MEASURED BY USING 10 REPEATED MEASUREMENTS. LINEARITY WAS MEASURED COVERING 10 POINTS, EVENLY SPREAD OVER THE RANGE. THE INSTRUMENT WAS SET ZERO BEFORE PERFORMING THE LINEARITY TEST. OFF-CENTER LOADING WAS MEASURED BY USING STANDARD WEIGHTS PLACED ON THE PAN AND MOVED TO VARIOUS POSITIONS ON THE PAN.

2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) STANDARD WEIGHT SET	E2	QK-I-151	C02250116	28-Jan-27
2) STANDARD WEIGHT	E2	15843	C02250117	29-Jan-27

3. THE CERTIFICATE IS VALID FOR THE ITEM CALIBRATED AS SHOWN ON THE DATE AND PLACE OF CALIBRATION ONLY.

4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.

5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-
- NATIONAL INSTITUTE OF METROLOGY (THAILAND)

RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

1. ZERO SETTING FUNCTION : NORMAL

2. TARE FUNCTION : NORMAL

3. REPEATABILITY OF READING AT 120 g WAS 0.000055 g

4. DEPARTURE FROM NOMINAL VALUE/ LINEARITY

NOMINAL VALUE (g)	BALANCE READING (g)	CORRECTION (g)	UNCERTAINTY (\pm g)
0.00	0.00000	0.00000	0.000065
0.02	0.01999	0.00001	0.000065
0.10	0.10001	-0.00001	0.000066
0.20	0.20001	-0.00001	0.000066
0.50	0.50002	-0.00002	0.000065
1.00	1.00003	-0.00003	0.000066
2.00	2.00001	-0.00001	0.000067
5.00	5.00002	-0.00002	0.000068
10.00	10.00000	0.00000	0.000070
20.00	20.00004	-0.00004	0.000078
50.00	50.00000	0.00000	0.00013
100.00	100.0001	-0.0001	0.00019
120.00	120.0002	-0.0002	0.00022

5. OFF CENTER LOADING ERROR



POINT	READING (g)
1	50.0000
2	50.0000
3	50.0000
4	50.0000
5	50.0000
OFF-CENTER LOADING	0.0000

NOTE: THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA
THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A
COVERAGE FACTOR $k=2$, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.


END OF CALIBRATION REPORT





CALIBRATION LABORATORY Co.,LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-G353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



CERTIFICATE OF CALIBRATION

FOR

NOMENCLATURE	VACUUM GAUGE
MANUFACTURER	HI-LIGHT
MODEL/TYPE	N/A
SERIAL NO.	N/A[64-220088-1]
CLID.NO.	212301422
JOB CONTROL NO.	240720076546

CUSTOMER S.P.S. CONSULTING SERVICE CO.,LTD.
7 SOI PHAHOLYOTHIN 24 ROAD., JOMPOL,
CHATUCHAK, BANGKOK 10900

DATE OF RECEIVED : 19 July 2025

DATE OF ISSUED: 24 July 2025

The report or calibration shall not be reproduced except in full without approval of the Calibration Laboratory Co., Ltd.

Calibrated By : Sittipong Pimdee
Calibration Engineer

Approved By : Mongkol Yotsoontorn
Authorized Signatory
24 July 2025



This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to the International System of Units (SI)

Certificate No. Q24076546


F3-011-05/12-23

page 1 of 3



CALIBRATION LABORATORY Co.,LTD.

211Q-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-Q353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



REPORT OF CALIBRATION

FOR

NOMENCLATURE	VACUUM GAUGE
MANUFACTURER	HI-LIGHT
MODEL/TYPE	N/A
SERIAL NO.	N/A [64-220088-1]
DATE OF CALIBRATION	23 July 2025
DUE DATE OF CALIBRATION	23 July 2026

ENVIRONMENT CONDITIONS

Temperature : (23 \pm 2) °C

Relative Humidity (55 \pm 10) %RH

PROCEDURE USED :

This instrument was calibrated under procedure No. CLC-CPPP-05 according to DKD-R 6-1 as calibration guidelines.

The calibration was performed by direct measurement with Document Process Calibrator and Pressure Module which maintained by the Calibration Laboratory Co., Ltd.

REFERENCE STANDARD USED :

Document Process Calibrator, Fluke Model 741B S/N 8295020 with Pressure Module Model 700PD5 S/N 89404505.

TRACEABILITY :

The measurements are traceable to International System of Units (SI), through National Institute of Metrology (Thailand).
Certificate No. MP-0040-24.

UNCERTAINTY :

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor of $k=2$. It has been evaluated according to the "Calibration of Pressure Gauges (DKD-R 6-1)" which provides a level of confidence approximately 95%.

Certificate No. Q24076546


F3-011-05/12-23

page 2 of 3



CAIBRATION LABORATORY Co., LTD.

2/1Q-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-D353-4 Fax:02-578-2672 www.caLaboratory.com E-mail:sale@cal-laboratory.com



CONDITION OF CALIBRATION ITEM :RECEIVED IN GOOD OPERATIONAL CONDITION

MEASUREMENT RESULTS: (X) without adjustment () adjustment

The DUC was exercised by applying a known pressure from its zero to full scale 1 times. Then 2 series of known gauge pressure were applied. The STD reading were recorded and the means value were reported in the table below.

CALIBRATION DATA

CORRECTION OF PRESSURE

DUC Test point (inHg)	STD Reading (kPa)		Conversion to inHg		Correction (inHg)	
	Up	Down	Up	Down	Up	Down
0	0.00	0.00	0.0	0.0	0.0	0.0
-5	-15.07	-15.10	-4.5	-4.5	+0.5	+0.5
-10	-32.50	-32.84	-9.6	-9.7	+0.4	+0.3
-15	-49.44	-49.77	-14.6	-14.7	+0.4	+0.3
-20	-66.70	-66.70	-19.7	-19.7	+0.3	+0.3
-25	-83.63	-83.97	-24.7	-24.8	+0.3	+0.2
-30	-100.39	-100.39	-29.6	-29.6	+0.4	+0.4

Uncertainty of measurement ± 0.2 inHg

Transmitting fluid : Air.

Technical Note. Conversion factor 1 kPa ; 0.2953003 inHg

Note. The Scope of Accredited ANAB Certificate No. ACDM-2814 Version 012 Page 43 of 67

This report is valid for the above stated instrument/s only.

End of Certificate

Certificate No. Q24076546

F3-011-05/ 12-23

Cert. No. : SP25026
Pages : 1 of 4

Calibration Certificate

Equipment : UV-VIS SPECTROPHOTOMETER
Manufacturer : PERKINELMER
Model : LAMBDA 25
Serial No.: 501S14123010
ID No.: SP03/58
Calibration Mode : WAVELENGTH ACCURACY
PHOTOMETRIC ACCURACY
STRAY LIGHT

Condition As Found : GOOD

Customer : S.P.S CONSULTING SERVICE CO., LTD.
7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN ROAD,
CHOMPHON SUB-DISTRICT, CHATUCHAK DISTRICT,
BANGKOK PROVINCE 10900 THAILAND.

Location : ORGANIC LABORATORY IV

Ambient Temperature : (22.9 ± 5) °C

Relative Humidity : (53.7 ± 25) %

Received Date : 22 AUGUST 2025

Calibration Date : 22 AUGUST 2025

Date of Issue : 25 AUGUST 2025

Calibrated by : Nitinun Srihawan

Approved by : *Wichok B.*
(Wichok Ekpongpradit)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

Cert. No. : SP25026
Job No. : VC68SP0019
Pages : 2 of 4

Calibration Method :

This instrument was calibrated by using on-site calibration procedure In-house method : CP-SP-01
The calibration procedure to direct measurement wavelength accuracy by using wavelength standard solution, Photometric accuracy by using absorbance standard filter and absorbance standard solution
The calibration procedure used was based on ASTM E275-01, ASTM E925-02

Condition of this result of calibration :

1. Certified reference materials

Material	Ref. type	Cell serial No.	Cert. No.	Due Date
Holmium liquid	RM-HL	29706	126461	24/10/2026
Didymium liquid	RM-DL	28912	126462	24/10/2026
Neutral density filter	RM-1N2N3N	13877	126457	24/10/2026
Potassium dichromate solutions	RM-0204060810	14204	126497	25/10/2026
Potassium Iodide solution	-	KI-0701-001	CI-0185-24	14/05/2026

2. This result of calibration was found accurate as shown on date and place of calibration only.

3. This certificate is traceable to the international system of unit maintained at :

3.1 The UK National Physical Laboratory (NPL)

Result of calibration : Wavelength Accuracy

(Without adjustment)

Material	Certified Values of Reference Material (nm)	UUC* Reading (nm)	Error (nm)	Uncertainty ± (nm)	k Factor
RM-HL	278.13	278.21	0.08	0.16	2.00
	361.25	361.39	0.14	0.16	2.00
	467.82	467.71	-0.11	0.16	2.00
	536.56	536.50	-0.06	0.16	2.00
	640.50	640.36	-0.14	0.16	2.00
RM-DL	740.09	739.85	-0.24	0.16	2.00
	864.94	865.12	0.18	0.16	2.00

UUC* = Unit Under Calibration

Cert. No. : SP25026
Job No. : VC68SP0019
Pages : 3 of 4

Result of calibration : Photometric Accuracy

Material	Wavelength (nm)	Filter S/N	Nominal Absorbance (A)	Certified Absorbance (A)	UUC* Reading Absorbance (A)	Error (A)	Uncertainty ± (A)	k Factor
Neutral Density glass filter	440.0	29381	0.5	0.5443	0.5413	-0.0030	0.0043	2.00
		29914	0.7	0.7484	0.7455	-0.0029	0.0054	2.00
		29360	1.0	1.0527	1.0535	0.0008	0.0032	2.00
	465.0	29381	0.5	0.4948	0.4922	-0.0026	0.0041	2.00
		29914	0.7	0.6906	0.6877	-0.0029	0.0050	2.00
		29360	1.0	0.9695	0.9709	0.0014	0.0031	2.00
	546.1	29381	0.5	0.5090	0.5068	-0.0022	0.0036	2.00
		29914	0.7	0.6985	0.6960	-0.0025	0.0041	2.00
		29360	1.0	0.9814	0.9825	0.0011	0.0031	2.00
	590.0	29381	0.5	0.5375	0.5353	-0.0022	0.0034	2.00
		29914	0.7	0.7256	0.7231	-0.0025	0.0037	2.00
		29360	1.0	1.0213	1.0219	0.0006	0.0032	2.00
	635.0	29381	0.5	0.5223	0.5202	-0.0021	0.0033	2.00
		29914	0.7	0.6927	0.6901	-0.0026	0.0036	2.00
		29360	1.0	0.9744	0.9750	0.0006	0.0032	2.00

UUC* = Unit Under Calibration

Cert. No. : SP25026
Job No. : VC68SP0019
Pages : 4 of 4

Result of calibration : Photometric Accuracy

(Without adjustment)

Material	Wavelength (nm)	Solution (mg/l)	Certified Absorbance (A)	UUC* Reading Absorbance (A)	Error (A)	Uncertainty ± (A)	k Factor
Potassium dichromate solutions	235.0	20	0.2415	0.2443	0.0028	0.0101	2.00
		40	0.4866	0.4871	0.0005	0.0115	2.00
		60	0.7415	0.7295	-0.0120	0.0067	2.00
		80	0.9854	0.9844	-0.0010	0.0071	2.00
		100	1.2444	1.2425	-0.0019	0.0073	2.00

UUC* = Unit Under Calibration

Condition of this result of calibration : Spectrophotometer PERKINELMER Model LAMBDA 25 S/N 501S14123010

Resolution of Wavelength Mode 0.1 nm
Resolution of Photometric Mode 0.001 A
Parameter Setting
Measurement Mode Wavelength, Absorbance
Wavelength Scan 190 nm - 1100 nm
Scanning Speed 7.5 nm/min
Band width(Wavelength) 1.0
Band width(Vis) 1.0
Band width(Uv) 1.0

Stray Light** UUC* Reading at 220.0 nm	
Transimission T(%)	Absorbance(A)
0.020	3.7032

**Specific Acceptance :
Transmission ≤ 1.0 T(%), Absorbance ≥ 2.0 A
**Stray light not TISI Accredited

The reported uncertainty is based on a standard uncertainty multiplied by a coverage factor k , providing a level of confidence of approximately 95%

End of Calibration Certificate



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

Personal Pump Calibration Report

Calibration Method : Dry Cal Primary Flowmeter

Model : Defender 510-H

S/N : 136833

Environmental Conditions

Temperature : 25 ± 3 °C
Pressure : 1010 ± 15 mmbar

Personal Pump Data				Calibration Data									
No.	Brand	Model	Serial No.	Date	Flow Rate (ml/min)						Value From Calibration Curve		
					Setting			Actual (Q std.)			y		
					1	2	3	1	2	3	y	R ²	
R01	SKC	224-PCXR4	602467	02/07/2025	1,000	1,500	2,000	997	1,510	2,008	1.008x - 10.783	1.000	
R02	SKC	224-PCXR4	626450	03/07/2025	1,000	2,000	3,000	999	1,498	1,993	0.991x + 9.648	1.000	
R03	SKC	224-PCXR4	691592	02/07/2025	1,000	1,500	2,000	1,005	1,501	1,998	1.006x - 13.328	0.999	
R04	SKC	224-PCXR4	691672	02/07/2025	1,000	1,500	2,000	999	1,493	2,002	1.001x - 3.364	1.000	
R05	SKC	224-PCXR4	798470	01/07/2025	1,000	1,500	2,000	996	1,509	2,001	1.009x - 19.500	0.999	
R06	SKC	224-PCXR4	798456	01/07/2025	1,000	1,500	2,000	997	1,498	1,998	1.004x - 8.490	1.000	
R07	SKC	224-PCXR4	798480	02/07/2025	1,000	1,500	2,000	998	1,494	2,001	1.006x - 11.786	1.000	
R08	SKC	224-PCXR4	883215	03/07/2025	1,000	1,500	2,000	1,009	1,505	2,006	1.001x + 0.899	1.000	
R09	SKC	224-PCXR4	034650	03/07/2025	1,000	1,500	2,000	996	1,508	1,999	1.008x - 17.223	0.999	
R10	SKC	224-PCXR4	091765	03/07/2025	1,000	1,500	2,000	999	1,495	1,998	1.002x - 2.097	1.000	
R11	SKC	224-PCXR4	091763	02/07/2025	1,000	1,500	2,000	1,002	1,498	2,002	1.010x - 18.889	0.999	
R12	SKC	224-PCXR4	091568	01/07/2025	1,000	1,500	2,000	997	1,506	2,001	1.004x - 7.711	1.000	
R13	SKC	224-PCXR4	091638	01/07/2025	1,000	1,500	2,000	1,006	1,498	1,997	0.991x + 13.423	1.000	
R14	SKC	224-PCXR4	091764	01/07/2025	1,000	1,500	2,000	994	1,505	1,996	1.007x - 17.870	0.999	
R15	SKC	224-PCXR8	529457	01/07/2025	1,000	1,500	2,000	1,005	1,504	1,994	0.995x + 5.338	1.000	
R16	SKC	224-PCXR8	529643	02/07/2025	1,000	1,500	2,000	1,000	1,499	1,997	1.000x - 2.577	1.000	
R17	SKC	224-PCXR8	529645	02/07/2025	1,000	1,500	2,000	996	1,507	1,993	1.004x - 12.365	0.999	
R18	SKC	224-PCXR8	566756	04/07/2025	1,000	1,500	2,000	995	1,498	1,996	0.997x + 0.819	1.000	
R19	SKC	224-PCXR8	566802	03/07/2025	1,000	1,500	2,000	1,003	1,499	2,002	1.012x - 22.181	0.999	
R20	SKC	224-PCXR8	529089	02/07/2025	1,000	1,500	2,000	994	1,502	1,996	1.001x - 5.166	1.000	
R21	SKC	224-PCXR8	665728	04/07/2025	1,000	1,500	2,000	999	1,497	2,001	1.003x - 8.170	1.000	
R22	SKC	224-PCXR8	707444	04/07/2025	1,000	1,500	2,000	1,004	1,504	2,006	1.005x - 6.228	1.000	
R23	SKC	224-PCXR8	761067	03/07/2025	1,000	1,500	2,000	996	1,498	1,996	0.998x - 1.215	1.000	
R24	SKC	224-PCXR8	707893	01/07/2025	1,000	1,500	2,000	999	1,508	1,995	1.002x - 7.415	0.999	
R25	SKC	224-PCXR8	761052	04/07/2025	1,000	1,500	2,000	1,004	1,501	1,997	0.992x + 12.437	1.000	
R26	SKC	224-PCXR8	707956	04/07/2025	1,000	1,500	2,000	1,005	1,505	2,009	1.011x - 15.349	0.999	
R27	SKC	224-PCXR8	707398	02/07/2025	1,000	1,500	2,000	997	1,506	1,995	1.000x - 5.721	1.000	
R28	SKC	224-PCXR8	707481	02/07/2025	1,000	1,500	2,000	1,005	1,503	1,993	1.001x - 6.976	0.999	
R29	SKC	224-PCXR8	707402	02/07/2025	1,000	1,500	2,000	1,004	1,496	1,992	0.995x + 1.966	1.000	
R30	SKC	224-PCXR8	093811	04/07/2025	1,000	1,500	2,000	1,003	1,497	1,999	0.998x + 1.047	1.000	
R31	SKC	224-PCXR8	093183	01/07/2025	1,000	1,500	2,000	1,004	1,505	1,995	0.996x + 6.964	1.000	
R32	SKC	224-PCXR8	671950	01/07/2025	1,000	1,500	2,000	998	1,503	1,998	1.000x + 1.382	1.000	
R33	SKC	224-PCXR4	626294	01/07/2025	1,000	1,500	2,000	999	1,507	1,997	1.006x - 14.223	0.999	
R34	SKC	224-PCXR4	626131	03/07/2025	1,000	1,500	2,000	1,005	1,501	1,991	0.993x + 7.387	1.000	
R35	SKC	224-PCXR8	707460	03/07/2025	1,000	1,500	2,000	999	1,499	1,999	0.997x + 3.684	1.000	
R36	SKC	224-PCXR8	707446	03/07/2025	1,000	1,500	2,000	1,005	1,501	2,001	1.009x - 16.388	0.999	
R37	SKC	224-PCXR8	707432	01/07/2025	1,000	1,500	2,000	1,000	1,498	2,003	1.000x - 0.875	1.000	
R38	SKC	224-PCXR8	707349	01/07/2025	1,000	1,500	2,000	998	1,492	2,002	1.003x - 6.681	1.000	
R39	SKC	224-PCXR8	761095	02/07/2025	1,000	1,500	2,000	1,003	1,499	2,001	1.001x - 0.859	1.000	

Calibrated by :

Adul Dangklom
(Mr. Adul Dangklom)

Approved by :

Peera Detudom
(Mr. Peera Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

Personal Pump Calibration Report

Calibration Method : Dry Cal Primary Flowmeter

Model : Defender 510-H

S/N : 136833

Environmental Conditions

Temperature : 25 ± 3 °C
Pressure : 1010 ± 15 mmbar

Personal Pump Data				Calibration Data									
No.	Brand	Model	Serial No.	Date	Flow Rate (ml/min)						Value From Calibration Curve		
					Setting			Actual (Q std.)			y		
					1	2	3	1	2	3	y	R ²	
R40	SKC	224-PCXR4	612753	02/07/2025	1,000	1,500	2,000	1,003	1,503	1,994	1.004x - 11.618	0.999	
R41	SKC	224-PCXR4	626140	02/07/2025	1,000	1,500	2,000	995	1,495	1,993	1.008x - 22.708	0.999	
R42	SKC	224-PCXR4	626463	02/07/2025	1,000	1,500	2,000	1,001	1,497	1,991	0.994x + 7.539	1.000	
R43	SKC	224-PCXR4	626129	01/07/2025	1,000	1,500	2,000	1,007	1,507	2,001	1.005x - 8.869	0.999	
R44	SKC	224-PCXR4	602753	01/07/2025	1,000	1,500	2,000	1,002	1,499	1,997	0.999x - 0.384	1.000	
R45	SKC	224-PCXR4	626137	02/07/2025	1,000	1,500	2,000	995	1,508	2,007	1.008x - 11.542	1.000	

Calibrated by :

Adul Dangklom
(Mr. Adul Dangklom)

Approved by :

Peera Detudom
(Mr. Peera Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

Rotameter Calibration Report (For Personal Pump High Flow Adjust)

Calibration Method : Dry Cal Primary Flowmeter

Model : Defender 510-H

S/N : 136164

Calibration Data

Rotameter Data			Calibration Data								
No.	Brand	Model	Date	Flow Rate (mL/min)						Value From Calibration Curve	
				Flow Rate (Reading)			Actual (Q std.)				
				1	2	3	1	2	3	y	R ²
H-R01	Dwyer	VFB-65	02/07/2025	500	1,000	2,000	498.8	1001.4	2005.7	0.996x + 4.876	1.000
H-R02	Dwyer	VFB-65	02/07/2025	500	1,000	2,000	501.6	1001.3	1997.6	0.997x + 5.643	1.000
H-R03	Dwyer	VFB-65	03/07/2025	500	1,000	2,000	499.3	1001.9	1990.3	0.998x + 3.307	0.999
H-R04	Dwyer	VFB-65	04/07/2025	500	1,000	2,000	501.3	997.3	2005.9	1.000x + 1.052	1.000
H-R05	Dwyer	VFB-65	02/07/2025	500	1,000	2,000	501.6	998.8	2005.5	1.003x - 1.210	1.000
H-R06	Dwyer	VFB-65	03/07/2025	500	1,000	2,000	500.9	1001.3	1990.6	0.997x + 5.814	0.999
H-R07	Dwyer	VFB-65	04/07/2025	500	1,000	2,000	501.9	1001.7	2009.2	0.999x - 1.217	1.000
H-R08	Dwyer	VFB-65	04/07/2025	500	1,000	2,000	499.0	998.4	2006.7	1.002x - 9.084	0.999
H-R09	Dwyer	VFB-65	02/07/2025	500	1,000	2,000	498.8	1000.5	1998.8	1.001x - 1.402	1.000
H-R10	Dwyer	VFB-65	02/07/2025	500	1,000	2,000	500.2	1000.6	2001.7	0.999x + 3.178	1.000

Calibrated by :

Adul Dangklom
(Mr. Adul Dangklom)

Approved by :

Mr. Peera Detudom



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

Rotameter Calibration Report (For Personal Pump High Flow Adjust)

Calibration Method : Dry Cal Primary Flowmeter

Model : Defender 510-H

S/N : 136164

Calibration Data

Rotameter Data			Calibration Data								
No.	Brand	Model	Date	Flow Rate (mL/min)						Value From Calibration Curve	
				Flow Rate (Reading)			Actual (Q std.)				
				1	2	3	1	2	3	y	R ²
H-R01	Dwyer	VFB-65	04/07/2025	500	1,000	2,000	500.4	999.6	2002.7	0.999x + 1.975	1.000
H-R02	Dwyer	VFB-65	04/07/2025	500	1,000	2,000	499.3	998.9	1998.1	1.000x - 0.723	1.000
H-R03	Dwyer	VFB-65	03/07/2025	500	1,000	2,000	500.5	998.7	1996.7	0.998x + 2.184	0.999
H-R04	Dwyer	VFB-65	02/07/2025	500	1,000	2,000	501.7	998.1	1993.3	1.000x - 2.212	0.999
H-R05	Dwyer	VFB-65	02/07/2025	500	1,000	2,000	499.2	997.5	1997.1	1.002x - 3.115	1.000
H-R06	Dwyer	VFB-65	02/07/2025	500	1,000	2,000	499.8	997.4	1993.2	1.001x - 4.572	0.999

Calibrated by :

Adul Dangklom
(Mr. Adul Dangklom)

Approved by :

Mr. Peera Detudom



บริษัท ไทยยูนิค จำกัด THAI UNIQUE CO., LTD.

80-82 ถนนประชาธิปไตย แขวงบางขุนพรหม เขตพระนคร กรุงเทพฯ 10200

80-82 Prachathipatai Rd., Bangkhunphrom, Pranakorn, Bangkok 10200

Tel. 0-2629-0191-6, 0-2280-1787, Fax. 0-2280-1788, E-mail : thawatt@thaiunique.com, Website : www.thaiunique.com

GAS CHROMATOGRAPH TEST CERTIFICATION

Certificate No. : SV0825/23032

Instrument Type : Gas Chromatography

Model : 3800

Serial Number : 00734

Organization : S.P.S. Consulting Service Co., Ltd.

Address : 7 Phahonyothin Soi 24 Phahonyothin Rd. Ladyao Chatuchak Bangkok 10900

Date : 02/08/2025

ELECTRONIC TEST

CPU	<input checked="" type="checkbox"/> PASS	<input type="checkbox"/> FAIL
DISPLAY & LED TEST	<input checked="" type="checkbox"/> PASS	<input type="checkbox"/> FAIL
VENT TEST	<input checked="" type="checkbox"/> PASS	<input type="checkbox"/> FAIL
KEY ECHO TEST	<input checked="" type="checkbox"/> PASS	<input type="checkbox"/> FAIL
DESTRUCTION RAM TEST	<input checked="" type="checkbox"/> PASS	<input type="checkbox"/> FAIL

RUN CHROMATOGRAM TEST

DETECTOR : Flame Ionization Detectors (FID Channel-Front)

INJECTOR : 1079 Injector

GC CONDITION:

Column	80 °C hold 1 min., rate 20 °C/min. to 200 °C hold 1min.
Injector	220 °C
Detector	300 °C
Column flow	5 mL/min
Makeup flow	25 mL/min
Air flow	300 mL/min
Hydrogen flow	30 mL/min

Column:Capillary Column CP sil 5 CB 0.25 ID x 15 M

Sample: 1 µL Injection FID Test Sample 0.218g/L C14,C15,C16 in hexane (diluted to 30ppm)

SENSITIVITY TEST: C15. (Area count) = 515,940 Counts.



บริษัท ไทยยูนิค จำกัด THAI UNIQUE CO., LTD.

80-82 ถนนประชาธิปไตย แขวงบางขุนพรหม เขตพระนคร กรุงเทพฯ 10200

80-82 Prachathipatai Rd., Bangkhunphrom, Pranakorn, Bangkok 10200

Tel. 0-2629-0191-6, 0-2280-1787, Fax. 0-2280-1788, E-mail : thawatt@thaiunique.com, Website : www.thaiunique.com

Detector Sensitivity (FID)

Detector Response	Result	Specification
Baseline Noise (µV)	2.40	≤ 50
Baseline Drift (%)	0.18	≤ 1
Sensitivity (S/N for C15)	19,716	≥ 1,024


Temperature Specification

Temperature	Set	Result	Specification
Column Oven (°C)	80	79	± 5
Injector (°C)	220	218	± 5
Detector (°C)	300	298	± 5
Incubator (°C)	60	N/A	± 5

Relative Standard Deviation % (%RSD)

Checkout Procedure	Result	Specification
Area C15 (%)	1.48	≤ 5
Retention Time C15 (%)	0.08	≤ 0.5

APPROVAL :

Signature: 

Engineer : Somchai Pohtongkam

Date : 02/08/2025



VARIAN

1/2

SERVICE DEPARTMENT

FR-SV-029 Rev. 04



VARIAN

2/2

SERVICE DEPARTMENT

FR-SV-029 Rev. 04



บริษัท ไทยยูนิค จำกัด

THAI UNIQUE CO., LTD.

80-82 ถนนประชาธิปไตย แขวงบางขุนพรหม เขตพระนคร กรุงเทพฯ 10200

80-82 Prachathipatai Rd., Bangkhunphrom, Pranakorn, Bangkok 10200

Tel. 0-2629-0191-6, 0-2280-1787, Fax. 0-2280-1788, E-mail : thawatt@thaiunique.com, Website : www.thaiunique.com

Results Integrated System Testing

Checkout Procedure	FID
Detector Position	Front
Inlet Type	1079 Injector
C15 Area 1	506,043
C15 Area 2	520,497
C15 Area 3	522,154
C15 Area 4	521,664
C15 Area 5	509,340
C15 Area Average	515,940
* % RSD (< 5 %)	1.48

* The precision specification should be less than 2.0 % RSD ** (Relative Standard Deviation) for an Auto sampler injection and less than 5 % for Manual injections. To calculate the %RSD, select the C15 peak area for each of the five (5) samples.

** (Relative Standard Deviation is determined by dividing the standard deviation by the average and multiplying by 100.)

$$\% \text{ RSD} = (\text{std.dev} / \text{avg}) * 100$$

Compliance	<input checked="" type="checkbox"/> Pass	<input type="checkbox"/> Fail
Performance by	Sankul P.	
Date	02/08/2025	



Comments			
Reviewed by	Wattana	Date	02/08/2025



บริษัท ไทยยูนิค จำกัด

THAI UNIQUE CO., LTD.

80-82 ถนนประชาธิปไตย แขวงบางขุนพรหม เขตพระนคร กรุงเทพฯ 10200

80-82 Prachathipatai Rd., Bangkhunphrom, Pranakorn, Bangkok 10200

Tel. 0-2629-0191-6, 0-2280-1787, Fax. 0-2280-1788, E-mail : thawatt@thaiunique.com, Website : www.thaiunique.com

Results Integrated System Testing

Checkout Procedure	FID
Detector Position	Front
Inlet Type	1079 Injector
C15 RT 1	3.874
C15 RT 2	3.880
C15 RT 3	3.875
C15 RT 4	3.872
C15 RT 5	3.878
C15 RT Average	3.876
* % RSD (< 0.5 %)	0.08

* The precision specification should be less than 0.5 % RSD ** (Relative Standard Deviation) for an Auto sampler injection and less than 0.5 % for Manual injections. To calculate the %RSD, select the RT C15 peak for each of the five (5) samples.

** (Relative Standard Deviation is determined by dividing the standard deviation by the average and multiplying by 100.)

$$\% \text{ RSD} = (\text{std.dev} / \text{avg}) * 100$$

Compliance	<input checked="" type="checkbox"/> Pass	<input type="checkbox"/> Fail
Performance by	Sankul P.	
Date	02/08/2025	



Comments			
Reviewed by	Wattana	Date	02/08/2025



VARIAN

1/1

SERVICE DEPARTMENT



VARIAN

1/1

SERVICE DEPARTMENT


Title :
Run File : e:\sps2025\blk001.run
Method File : c:\star\data\tu\2025\cal fid.mth
Sample ID : blk

Injection Date: 2/8/2568 12:01 Calculation Date: 2/8/2568 12:33

Operator : watsamon Detector Type: 3800 (10 Volts)
Workstation: GC-LAB Bus Address : 44
Instrument : Sample Rate : 10.00 Hz
Channel : Front = FID Run Time : 20.005 min

** LC Workstation Version 6.20 ** 02511-7390-ae7-0265 **

Chart Speed = 1.13 cm/min Attenuation = 1 Zero Offset = 50%
Start Time = 0.000 min End Time = 20.005 min Min / Tick = 1.00

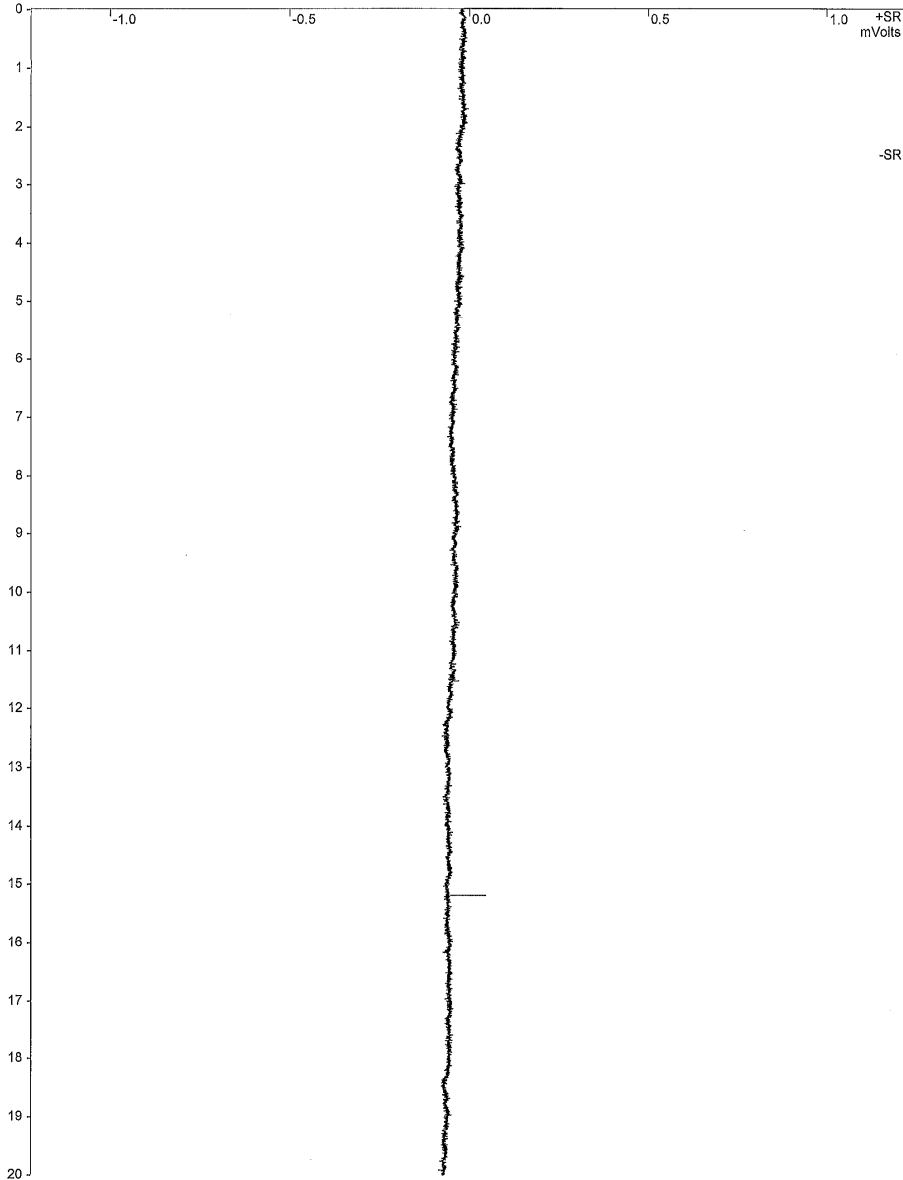

Print Date: Sat Aug 02 15:09:03 2025 Page 1 of 1

Title :
Run File : e:\sps2025\blk001.run
Method File : c:\star\data\tu\2025\cal fid.mth
Sample ID : blk

Injection Date: 2/8/2568 12:01 Calculation Date: 2/8/2568 12:33

Operator : watsamon Detector Type: 3800 (10 Volts)
Workstation: GC-LAB Bus Address : 44
Instrument : Sample Rate : 10.00 Hz
Channel : Front = FID Run Time : 20.005 min

** LC Workstation Version 6.20 ** 02511-7390-ae7-0265 **

Run Mode : Analysis
Peak Measurement: Peak Area
Calculation Type: External Standard

Peak No.	Peak Name	Result ()	Ret. Time (min)	Time Offset (min)	Area (counts)	Sep. Code	Width 1/2 (sec)	Status Codes
Totals:		0.0000		0.000	0			

Total Unidentified Counts : 0 counts

Detected Peaks: 0 Rejected Peaks: 0 Identified Peaks: 0

Multiplier: 1 Divisor: 1 Unidentified Peak Factor: 0

Baseline Offset: -14 microVolts LSB: 1 microVolts

Noise (used): 24 microVolts - monitored before this run

Manual injection

Data Handling: No peaks


Title :
Run File : e:\sps2025\fidstd001.run
Method File : c:\star\data\tu\2025\cal fid.mth
Sample ID : fidstd

Injection Date: 2/8/2568 12:34 Calculation Date: 2/8/2568 13:26

Operator : watsamon Detector Type: 3800 (10 Volts)
Workstation: GC-LAB Bus Address : 44
Instrument : Sample Rate : 10.00 Hz
Channel : Front = FID Run Time : 7.993 min

** LC Workstation Version 6.20 ** 02511-7390-ae7-0265 **

Chart Speed = 2.83 cm/min Attenuation = 79 Zero Offset = 2%
Start Time = 0.000 min End Time = 7.993 min Min / Tick = 1.00

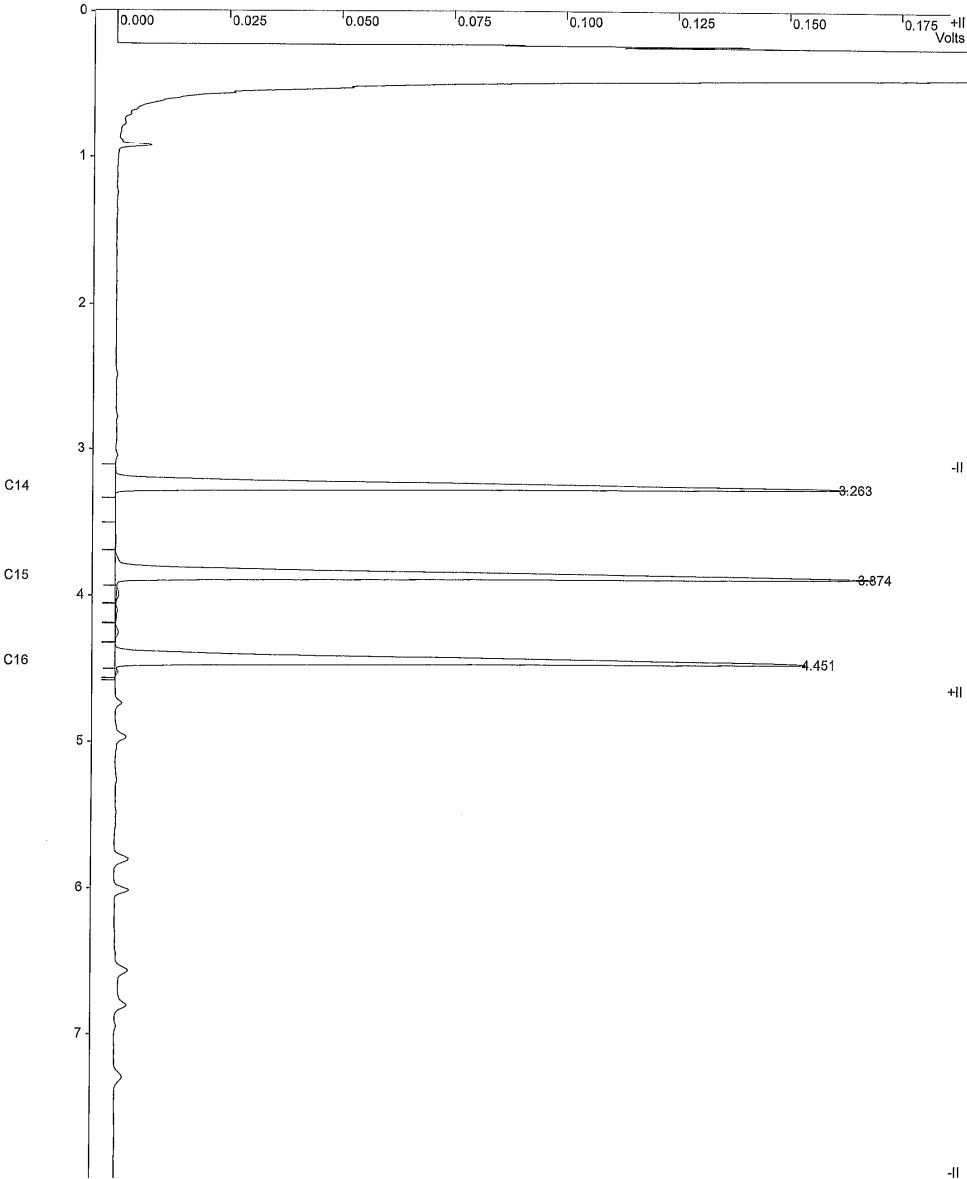

Print Date: Sat Aug 02 15:10:09 2025 Page 1 of 1

Title :
Run File : e:\sps2025\fidstd001.run
Method File : c:\star\data\tu\2025\cal fid.mth
Sample ID : fidstd

Injection Date: 2/8/2568 12:34 Calculation Date: 2/8/2568 13:26

Operator : watsamon Detector Type: 3800 (10 Volts)
Workstation: GC-LAB Bus Address : 44
Instrument : Sample Rate : 10.00 Hz
Channel : Front = FID Run Time : 7.993 min

** LC Workstation Version 6.20 ** 02511-7390-ae7-0265 **

Run Mode : Calibration
Peak Measurement: Peak Area
Calculation Type: External Standard
Level : 1

Peak No.	Peak Name	Ret. Time (min)	Time Offset (min)	Area (counts)	Sep. Code	Width 1/2 (sec)	Status Codes
1	C14	3.263	0.002	458627	BB	2.7	
2	C15	3.874	0.002	506043	VV	2.8	
3	C16	4.451	0.001	460610	VB	2.8	
Totals:			0.005	1425280			

Total Unidentified Counts : 0 counts

Detected Peaks: 8 Rejected Peaks: 5 Identified Peaks: 3

Multiplier: N/A Divisor: N/A Unidentified Peak Factor: 0

Baseline Offset: 6 microVolts LSB: 1 microVolts

Noise (used): 2 microVolts - monitored before this run

Manual injection

Sample ID: fid std


Operator (Inj): watsamon
Injection Date: 02/08/2025
Calc Date: 02/08/2025
Run Time (min): 7.993
Workstation: GC-LAB
Instrument (Inj):

**VARIAN**

Run Mode: Calibration
Peak Measurement: Peak Area
Calculation Type: External Std.

e:\sps2025\fidstd001.run

A = FID 10 V RESULTS

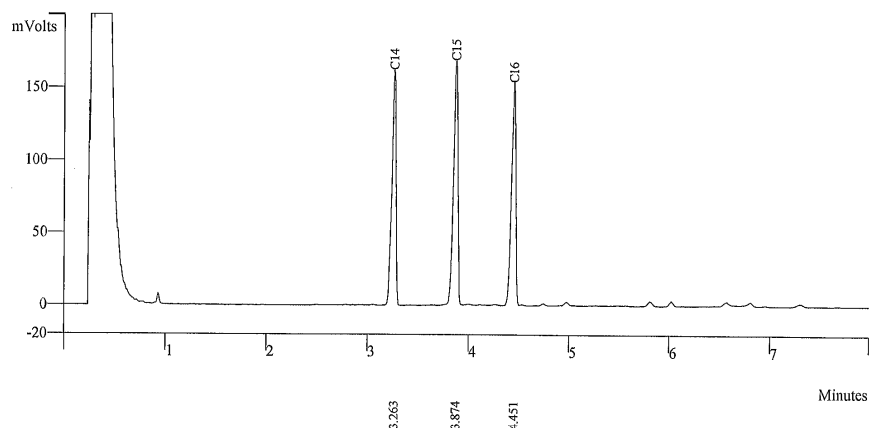

Peak No	Peak Name	Result ()	Ret Time (min)	Peak Area (counts)	Sep. Code	Width 1/2 (sec)
1	C14	0.0000	3.263	458627	BB	2.7
2	C15	0.0000	3.874	506043	VV	2.8
3	C16	0.0000	4.451	460610	VB	2.8
Totals		0.0000		1425280		



Sample ID: fid std


Operator (Inj): watsamon
Injection Date: 02/08/2025
Calc Date: 02/08/2025
Run Time (min): 7.993
Workstation: GC-LAB
Instrument (Inj):

**VARIAN**

Run Mode: Calibration
Peak Measurement: Peak Area
Calculation Type: External Std.

e:\sps2025\fidstd002.run

A = FID 10 V RESULTS

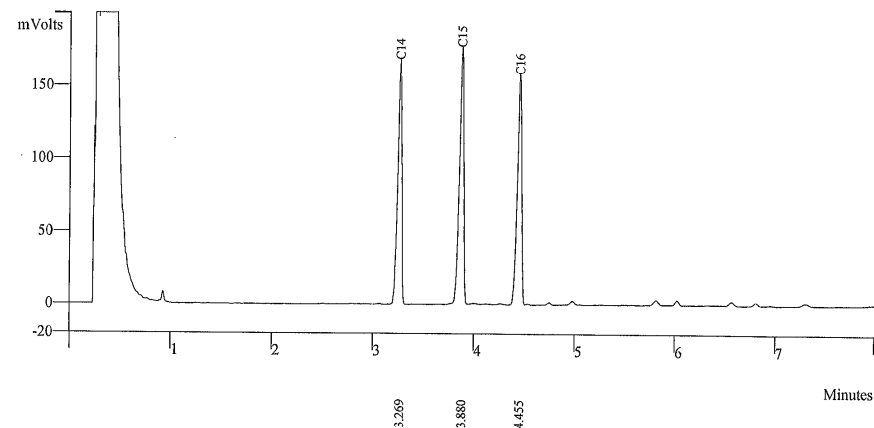

Peak No	Peak Name	Result ()	Ret Time (min)	Peak Area (counts)	Sep. Code	Width 1/2 (sec)
1	C14	0.0000	3.269	472338	BB	2.6
2	C15	0.0000	3.880	520497	VV	2.7
3	C16	0.0000	4.455	471916	VB	2.8
Totals		0.0000		1464751		



Sample ID: fid std


Operator (Inj): watsamon
Injection Date: 02/08/2025
Calc Date: 02/08/2025
Run Time (min): 7.993
Workstation: GC-LAB
Instrument (Inj):

**VARIAN**

Run Mode: Calibration
Peak Measurement: Peak Area
Calculation Type: External Std.

e:\sps2025\fidstd003.run

A = FID 10 V RESULTS

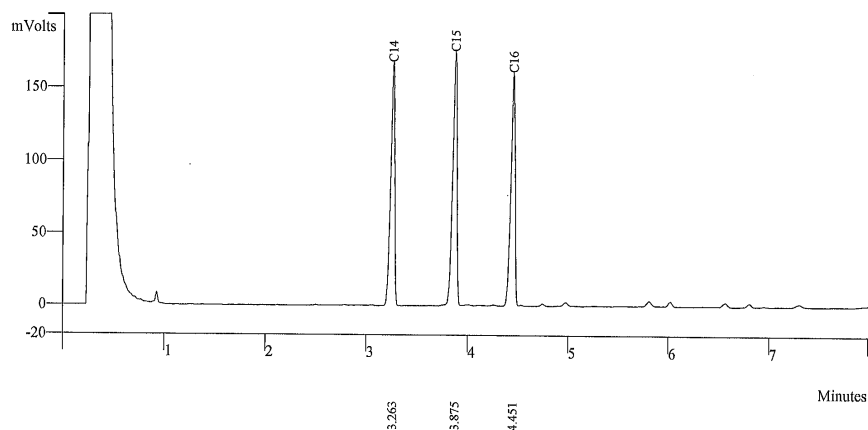

Peak No	Peak Name	Result ()	Ret Time (min)	Peak Area (counts)	Sep. Code	Width 1/2 (sec)
1	C14	0.0000	3.263	469265	BB	2.6
2	C15	0.0000	3.875	522154	VV	2.8
3	C16	0.0000	4.451	478526	VB	2.8
Totals		0.0000		1469945		



Sample ID: fid std


Operator (Inj): watsamon
Injection Date: 02/08/2025
Calc Date: 02/08/2025
Run Time (min): 7.993
Workstation: GC-LAB
Instrument (Inj):

**VARIAN**

Run Mode: Calibration
Peak Measurement: Peak Area
Calculation Type: External Std.

e:\sps2025\fidstd004.run

A = FID 10 V RESULTS

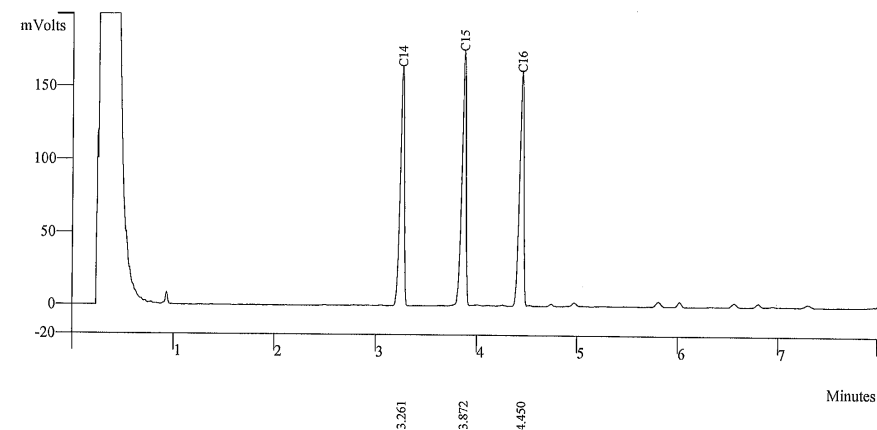

Peak No	Peak Name	Result ()	Ret Time (min)	Peak Area (counts)	Sep. Code	Width 1/2 (sec)
1	C14	0.0000	3.261	468907	BB	2.7
2	C15	0.0000	3.872	521664	VV	2.8
3	C16	0.0000	4.450	478772	VB	2.8
Totals		0.0000		1469343		



Sample ID: **fid std**


Operator (Inj): watsamon
Injection Date: 02/08/2025
Calc Date: 02/08/2025
Run Time (min): 7.993
Workstation: GC-LAB
Instrument (Inj):



Run Mode: Calibration
Peak Measurement: Peak Area
Calculation Type: External Std.

e:\sps2025\fidstd005.run

A = FID 10 V RESULTS

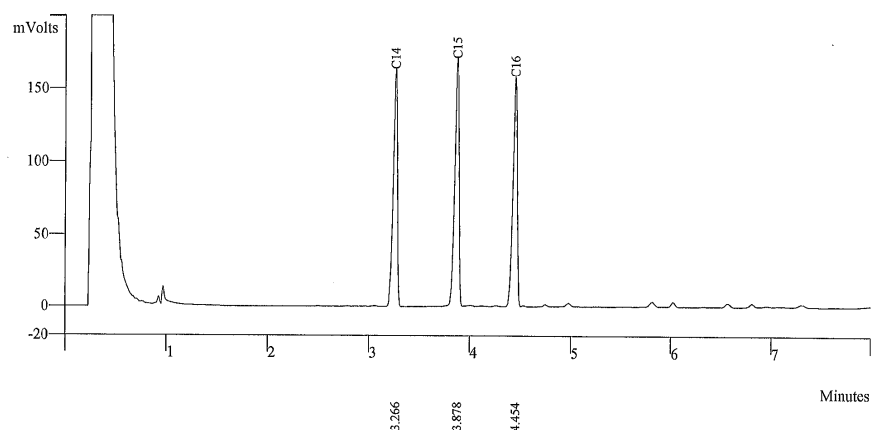

Peak No	Peak Name	Result ()	Ret Time (min)	Peak Area (counts)	Sep. Code	Width 1/2 (sec)
1	C14	0.0000	3.266	459351	BB	2.6
2	C15	0.0000	3.878	509340	VV	2.8
3	C16	0.0000	4.454	468353	VB	2.8
Totals		0.0000		1437044		



THAI UNIQUE CO.,LTD.


1 Of 1

Print Date: 02 Aug 2025 15:12:58
Calibration Curves Report
File: e:\sps2025\cal fid.mth
Detector: 3800 GC, Address: 44, Channel ID: Front

C14

External Standard Analysis
Curve Type: Linear
Origin: Force
 $y = +1.552325e+004x$


Resp. Fact. RSD: 1.347%
Coeff. Det.(r²): 0.999130

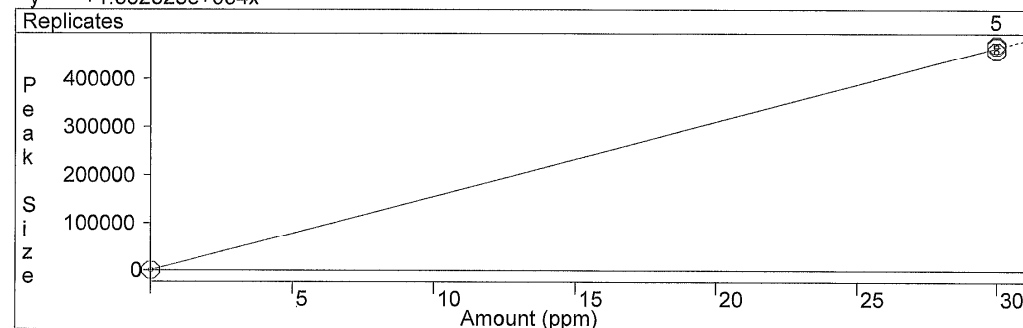

C15

External Standard Analysis
Curve Type: Linear
Origin: Force
 $y = +1.719798e+004x$


Resp. Fact. RSD: 1.481%
Coeff. Det.(r²): 0.998948

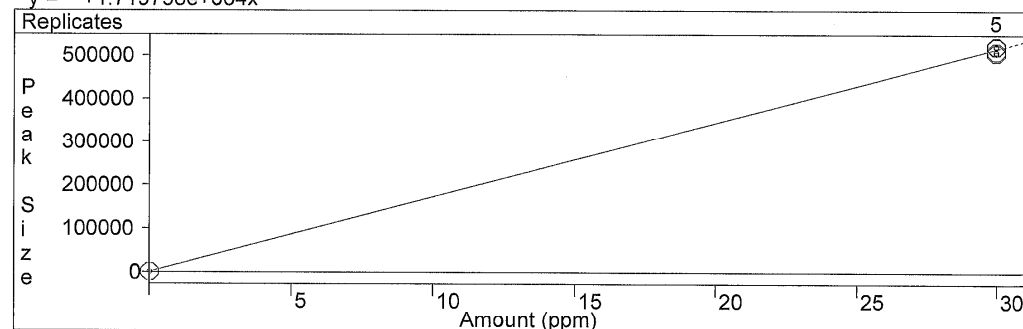

C16

External Standard Analysis
Curve Type: Linear
Origin: Force
 $y = +1.572118e+004x$

Resp. Fact. RSD: 1.611%
Coeff. Det.(r²): 0.998756

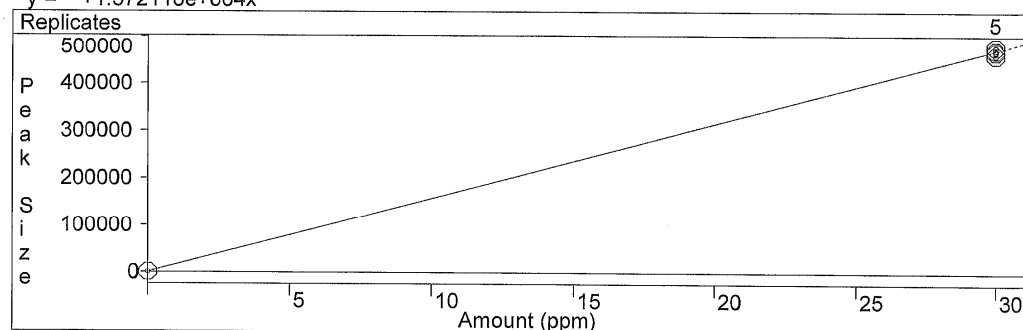

CERTIFICATE

This is to certify, that

Somchai Pohthongkham

has participated the course

Basic GC and Sampler training

Date: **24 – 27 May 2004**

Location: **Middelburg**

Instructor: **W.J. Buys**

Signature instructor: 



Varian Analytical Instruments
Varian Chrompack International BV
Herculesweg 8
P.O. Box 8033
4330 EA Middelburg
The Netherlands
Tel.: +31 118 671000
Fax: +31 118 631118
www.varianinc.com



WK Electric Co., Ltd.

68/242 Moo 5, Sawalpracharaj Rd., Tumbol Ladsawai, Amphur Lamlukka, Pathumthani 12150

Tel. +66 2993 4773, +66 2153 7132-3 Fax. +66 2994 5509 E-mail : wk.calibrations@gmail.com www.wk-etc.com



Certificate of Calibration

Certificate No.: WK2412-053-1

Page 1 of 2

Customer : THAI UNIQUE CO., LTD.
80-82 Prachathipatai Rd., Bangkokphrom,
Pranakorn, Bangkok 10200

Instrument	: AMD Flow Meter	Ambient Temperature	: (23 ± 2) °C
Manufacturer	: Agilent Technologies	Humidity	: (50 ± 15) %RH
Model	: G6691A	Received Date	: 4-Dec-24
Serial No.	: MY16470347	Calibrated Date	: 11-Dec-24
Identity No.	: SV-DF-001	Issued Date	: 13-Dec-24
Range	: 0 ml/min to 750 ml/min	Calibrated Location	: In Lab
Resolution	: See to Data		
Calibration Method	: CP-WK-M10		

Reference standard instruments :

Instrument	Serial No.	Certificate No.	Due Date	Traceability to
Flow Calibrator	140215-134	L202304114-001	18-Apr-25	MIT
Primary Flow Calibrator	1107-S	WK2405-049-5	22-May-25	WK Electric Co., Ltd.


MIT : Miracle International Technology Co., Ltd.

This result calibrate was found accurate as shown on date place of calibrate only
This certificate is traceability to the International System of Unit (SI)

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k=2$, providing a level of confidence approximately 95%

Calibrated by : Mr.Thippatai Mungpungklang

Approved by :


Ms. Budsagorn Patcha

Authorized Signatory

This certificate may not be reproduced except in full unless permission for the reproduction has been obtained in writing from the laboratory.



Measuretronix Limited
2425/2 Lat Phrao Road, Saphan Song
Wangthonglang, Bangkok 10310, Thailand
Phone : 0-2514-1000, 0-2514-1234
Fax : 0-2514-0001, 0-2514-0003
Website : www.measuretronix.com



Certificate of Calibration

Certificate Number : LF25-0305
Equipment : Thermometer
Manufacturer : Fluke
Model : 51
Serial Number : 5910857
Asset Number : 5910857
Customer : Thai Unique Co., Ltd.
80-82 Prachathipatai Road,
Bangkhunphrom, Pranakorn,
Bangkok 10200
Date of Calibrate : 6-Jun-2025
Date of Issue : 6-Jun-2025

This calibration certificate documents the traceability to national standards, which realize the units of measurement according to the International System of Units (SI).

This calibration certificate applies only to the item identified and shall not be reproduced other than in full, without specific written approval by Measuretronix Cal-Lab. Calibration certificates without signature are not valid.

The measurements marked with an asterisk () in this certificate are outside our range of accreditation. They have been included for completeness.*

The Calibration interval (Cal.Due) is the responsibility of the end user.

Calibrated by

Samak

Mr. Samak Uaonkaonoi
Metrology Technician

Approved by

Miss Juthamas Sukhathairun

Miss Juthamas Sukhathairun
Cal-Lab Manager



Agilent Technologies

Certificate of Analysis

FID-TCO Performance Evaluation Sample Kit

Agilent Part Number: 5080-8842, 18710-60170

Sample Lot Number: 0006750304

This analytical reference material was manufactured and verified in accordance with an ISO 9001 registered quality system, and the analyte concentrations were verified by an ISO 17025 accredited laboratory. The certified value for each analyte was determined gravimetrically.

Concentrations:		
n-tetradecane	0.218 g/L ($\pm 0.5\%$)	0.033 w/w %
n-pentadecane	0.218 g/L ($\pm 0.5\%$)	0.033 w/w %
n-hexadecane	0.218 g/L ($\pm 0.5\%$)	0.033 w/w %


Solvent: hexane

Calibrated Class A glassware and clean bottles were used in the manufacture of this standard. Balances used in the manufacture of this standard are calibrated with weights traceable to NIST in compliance with ANSI/NCCL Z-540-1 and ISO 9001.

Purities:	
n-tetradecane	99.6%
n-pentadecane	99%
n-hexadecane	99.5%
hexane	99%

Typical Analytical Spectrum or Chromatography

GC Chromatography – n-tetradecane, n-pentadecane, and n-hexadecane in hexane

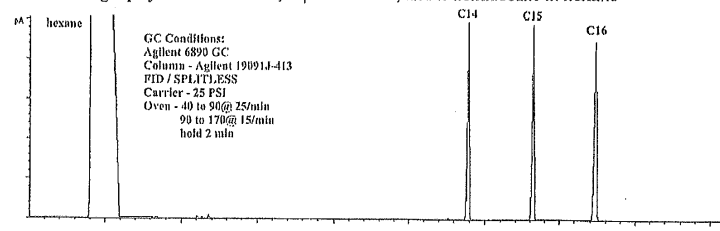

Date of release: 30 June 2023

Date of expiration: 31 July 2025

Monica Bourgeois
Monica Bourgeois
QMS Representative

เอกสารแนบ 5-3

เอกสารสอบเทียบเครื่องมือการตรวจวัดระดับเสียงในบรรยากาศ



THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-68/0220

MTC No. EEL. BP. 44/0268

CALIBRATION CERTIFICATE

Submitted by : S.P.S.Consulting Service Co.,Ltd.

Address : 7 Soi Phaholyothin 24, Phaholyothin Road, Jompol, Chatuchak, Bangkok 10900.

Calibrated at : Electrical and Electronic Standards Laboratory, Industrial Metrology and Testing Service Centre.
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Rd., Muang, Samutprakan 10280.

Instrument Calibrated :

Description : Sound Calibrator

Manufacturer : ACO

Model : 2127

Serial No. : 130006

Ambient Environment

Temperature : (23 ± 3) °C

Relative Humidity : (50 ± 15) %

Ambient Pressure : (101.325 ± 1.500) kPa

Standards used : 1. Digital Function Synthesizer NF Electronic DF-193A S/N 122037.

2. Measuring Amplifier Bruel&Kjaer 2636 S/N 1537484.

3. Programmable Attenuator Tamagawa TPA-303A S/N OF 2214.

4. Digital Multimeter Agilent 34401A S/N MY44005560.

5. Pressure Transmitter Vaisala PTB202AD S/N T0650001.

6. Audio Analyzer Panasonic VP-7722A S/N 041477D122.

7. Condenser Microphone B&K 4180 S/N 2889871.

Calibration Procedure: CP-102-04 based on IEC 60942-2003; The sound pressure level generated by sound calibrator under test shall be measured by standard microphone using an insert voltage technique.

This instrument has been calibrated against standards maintained at Electrical and Electronic Standards Laboratory (EEL), which are traceable to the International System of Units through the National Institute of Metrology (Thailand).

The information on actual reading is attached herewith and the uncertainty limits quoted refer to the measured values only.

Date of Receipt : 19 Feb. 2025

Date of Calibration : 21 Feb. 2025

1 / 2

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.5



THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-68/0220

MTC No. EEL. BP. 44/0268

The reported expanded uncertainty is based upon a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%.

Nominal Output of Unit Under Test = 94 dB re 20μPa at 1000 Hz

Acoustic Output in dB re 20μPa, Corrected to Reference Conditions: 101.325 kPa, 23.0 °C and 50 %RH.

1. Sound Pressure Level

Standard Microphone Type	Measured Sound Pressure Level (dB)	Deviated value (dB)	Uncertainty (dB)	Tolerance limit IEC60942:2003 Class 1
1/2 inch Bruel&Kjaer 4180	93.81	-0.19	± 0.10	±0.40 dB

2. Frequency

Standard Microphone Type	Measured Frequency (Hz)	Deviated value (Hz)	Uncertainty (Hz)	Tolerance limit IEC60942:2003 Class 1
1/2 inch Bruel&Kjaer 4180	999.9	-0.1	± 1.5	±1.0%

3. Total Distortion

Standard Microphone Type	Measured Total Distortion (%)	Uncertainty (%)	Tolerance limit IEC60942:2003 Class 1
1/2 inch Bruel&Kjaer 4180	0.95	± 0.50	±3.0%

Note : 1. No adjustment.

2. The calibrator pressure correction was not included.

3. The microphone volume correction was not included.

Calibrated by :

(Mr. Weerachai Deechaiyae)

Approved by :

(Mr. Prawate Kluaypa)
Director

Electrical and Electronic Standards Laboratory

Industrial Metrology and Testing Service Centre

Date of Calibration : 21 Feb. 2025

Date of Issue : 24 Feb. 2025

Ref : 2011268021900739001

End of Certificate

2 / 2

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.5

Head Office

35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9009

Office/Laboratory

668 Mu 2 Tambon Bangpoornai, Amphoe Muang Samutprakan,
Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtc@tistr.or.th Website : www.tistr.or.th

Office

196 Phahonyothin Road, Ladyao, Chatuchak,
Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827

Head Office

35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9009

Office/Laboratory

668 Mu 2 Tambon Bangpoornai, Amphoe Muang Samutprakan,
Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtc@tistr.or.th Website : www.tistr.or.th

Office

196 Phahonyothin Road, Ladyao, Chatuchak,
Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72. Fax : (662) 513-4221. E-mail : sale@spscon.com, www.spscon.com

Noise R_502/25

Sound Level Meter Calibration Report

Acoustic Calibrator Data

Brand	ACO	Number	AC 03/56
Model	2127	Serial No.	130006
Calibration Range	94 dB, 1000 Hz	Last Calibration	21 February 2025
		Due Date	21 February 2026

Calibration Data

Sound Level Meter Data				Calibration Data		
SLM No.	Brand	Model	Serial No.	Date	Actual Reading [dB]	
					Before Adjustment	After Adjustment
ACO-R02	ACO	6236	00132029	19 August 2025	93.9	93.9
ACO-R48	ACO	6236	00192060	19 August 2025	93.9	93.9
Acoustic Certified Value : Thailand Institute of Scientific and Technological Research (TISTR)					93.81 ± 0.10 dB	

Calibrated by :

Adul Dangklom
(Mr. Adul Dangklom)

Approved by :

Peera Detudom
(Mr. Peera Detudom)

เอกสารแนบ 5-4

เอกสารสอบเทียบเครื่องมือการตรวจวิเคราะห์คุณภาพน้ำทิ้ง



CALIBRATION LABORATORY Co.,LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



CERTIFICATE OF CALIBRATION

FOR

NOMENCLATURE : pH METER
MANUFACTURER : HANNA
MODEL / TYPE : HI3512/HI1332/HI7662-T
SERIAL NO. : 08685754/11250B7M/092806BN[PH04/56]
CLID. NO. : 272501562
JOB CONTROL NO. : 250617070523
CALIBRATION SERVICE : ☒ IN-LABORATORY ☐ ON-SITE

CUSTOMER : S.P.S. CONSULTING SERVICE CO., LTD.
7 SOI PHAHOLYOTHIN 24 ROAD, JOMPOL,
CHATUCHAK, BANGKOK 10900

DATE OF RECEIVED : 17 June 2025

DATE OF ISSUED : 20 June 2025

The report of calibration shall not be reproduced except in full without approval of the Calibration Laboratory Co., Ltd.

Calibrated By : Sukgasem Seehanart
Wenick Inchaistri
Calibration Engineer

Approved By : Mongkol Yotsoontorn
Authorized Signatory
20 June 2025



This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to the International System of Units (SI)

Certificate No. Q25070523

F3-011-05/12-23

page 1 of 4



@clccalibration



CALIBRATION LABORATORY Co.,LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



REPORT OF CALIBRATION

FOR

NOMENCLATURE : pH METER
MANUFACTURER : HANNA
MODEL / TYPE : HI3512/HI1332/HI7662-T
SERIAL NO. : 08685754/11250B7M/092806BN[PH04/56]
DATE OF CALIBRATION : 18 June 2025

ENVIRONMENT CONDITIONS :

Temperature : $(25 \pm 2.5) ^\circ\text{C}$ Relative Humidity : $(50 \pm 15) \% \text{ RH}$

PROCEDURE USED :

This instrument was calibrated under procedure No. CLC-CPCH-01 [pH Meter]. The calibration was performed by direct measurement with Certified Reference Material (CRM).

This instrument was calibrated under procedure No. CLC-CPTH-04 [Temperature] based on ASTM E 644-04 as calibration guidelines. The calibration was performed by using Calibration Bath, Precision Thermometer and IPRT which maintained by the Calibration Laboratory Co., Ltd.

REFERENCE STANDARD USED :

1. pH Standard Solution, NIMT TRM CODE TRM-S-2003, TRM CODE TRM-S-2007.
2. pH Standard Solution, Control Company Catalog Number 06664260,11754256, Lot Number CC787362.
3. Calibration Bath, Kambic Model OB-22/2 ULT S/N. 17115653.
4. Precision Thermometer, ASL Model F250 S/N. 1334023800.
5. IPRT, Wika Model CTP5000-250-D S/N. PO00043543-1-10-1.

Certificate No. Q25070523

F3-011-05/12-23

page 2 of 4



@clccalibration



CALIBRATION LABORATORY Co.,LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



TRACEABILITY :

1. The measurements are traceable to International System of Units (SI) , through National Institute of Metrology (Thailand).
Lot Number. 080124 , 120124. Due Date 23 January 2026.
2. The measurements are traceable to International System of Units (SI) , through Control Company.
Certificate No. 4281-14495731 , Due Date 27 September 2025.
3. The measurements are traceable to International System of Units (SI) , through Calibration Laboratory Co., Ltd.
Certificate No. Q24120999, Due Date 26 November 2025.
4. The measurements are traceable to International System of Units (SI) , through Thailand Institute of Scientific and Technological Research (TISTR). Certificate No. PSL-T 1042/67, Due Date 16 October 2025.
5. The measurements are traceable to International System of Units (SI) , through National Institute of Metrology (Thailand).
Certificate No. TT-0146-24, Due Date 28 October 2025.

UNCERTAINTY :

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor complies with the table which for a normal distribution corresponds to a coverage probability of approximately 95 %.

It has been evaluated according to the "Evaluation of the Uncertainty of Measurement in Calibration (EA-4/02 M:2022)"

Certificate No. Q25070523
F3-011-05/12-23

page 3 of 4



CALIBRATION LABORATORY Co.,LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



CONDITION OF CALIBRATION ITEM : RECEIVED IN GOOD OPERATIONAL CONDITION

MEASUREMENT RESULTS : (X) without adjustment () adjustment

The table in the following gives the calibration results and associated measurement uncertainties of pH meter.

CALIBRATION DATA

1. pH METER RESULT @ 25 °C

Standard pH Buffer Solution (pH)	pH Meter Reading (pH)	pH Meter Reading (mV)	Correction (pH)	Uncertainty of pH Measurement (\pm pH)	k Factor
4.003	4.005	168.2	-0.002	0.010	2,00
7.005	7.010	-8.1	-0.005	0.013	2,00
10.015	10.010	-177.7	+0.005	0.014	2,00

Technical Note. Setting function CAL 3 point (4,7,10).

Note. The Scope of Accredited ANAB Certificate No. ACDM-2814 Version 015 Page 4 of 68

2. TEMPERATURE RESULT

Immersion depth (mm)	Actual Temperature (°C)	DUC Reading (°C)	Correction (°C)	Uncertainty \pm (°C)
100	25.00	25.0	0.00	0.07

Technical Note. Type of sensor : Thermistor

Probe \varnothing 3 mm

Materials : Metal Sheath.

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor of $k = 2,00$.

Note. The Scope of Accredited ANAB Certificate No. ACDM-2814 Version 015 Page 56 of 68

This report is valid for the above stated instrument/s only.

End of Certificate

Certificate No. Q25070523
F3-011-05/12-23

page 4 of 4



CERT.No.: HS-W015C

Certificate of Calibration

Calibration Date : 18 Mar 25

Submitted by : S.P.S CONSULTING SERVICE CO.,LTD

7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol,

Chatuchak, Bangkok, Thailand 10900

Avg Room Temp : 20 °C

Avg Water Temp : 20 °C

Air Pressure : 760.00 mmHg

Salinity : 0 ppt

Model : YSI 5000

S/N : 15B100751

Probe : YSI 5010

S/N : 22D100097

ID NO. : -

Air Temp ref : S/N. F8065C26

Barometric ref : S/N. F8065C26

Water Temp ref : -

ID NO. HS001

Technician : Kittipong M.

Calibration Details

Calibration Point	100% air sat. (@20 °C, DO = 9.09 mg/l)	(status)	(status)
Measurement 1 (mg/l)	9.08	(PASS)	-
Measurement 2 (mg/l)	9.08	(PASS)	-
Measurement 3 (mg/l)	9.08	(PASS)	-
Measurement 4 (mg/l)	9.07	(PASS)	-
Measurement 5 (mg/l)	9.07	(PASS)	-
Measurement 6 (mg/l)	9.07	(PASS)	-
Measurement 7 (mg/l)	9.07	(PASS)	-
Measurement 8 (mg/l)	9.07	(PASS)	-
Measurement 9 (mg/l)	9.07	(PASS)	-
Measurement 10 (mg/l)	9.07	(PASS)	-

Mean Measurement	9.07	mg/l	-	-
Inaccuracy	0.02	mg/l	-	-

Overall Status (PASS)

Manufacturer Specification


Accuracy = +/- 0.02 mg/l

- 1) This certificate is issued based on the result that are found as shown on date and place of test only.
- 2) The calibration procedure followed in accordance with Harikul Science Co., Ltd.
- 3) This result shall not be used for advertising purpose.



Technician Signature

(Kittipong Maekwong)



Laboratory Manager

(Natenapha Pisatkunchon)

**QUALITY CALIBRATION CO., LTD.**

235 Petchkasem 63/2 Road, Laksong, Bangkai, Bangkok 10160

Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

www.qcalibration.com

CERTIFICATE No : 25T0520

REFERENCE No : 75853-1

PAGE : 1 OF 2

Certificate of Calibration

EQUIPMENT : COD REACTOR

MANUFACTURER : HACH

MODEL : DRB 200

SERIAL No : 15110C0497

ID No : DRB 05/59

CONDITION AS RECEIVED : USED ITEM

SUBMITTED BY : S.P.S. CONSULTING SERVICE CO., LTD.
7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN RD.,
JOMPOL, CHATUCHAK, BANGKOK 10900

CALIBRATED BY : CHAICHARN CH.

CALIBRATION DATE : 27-Jan-25

APPROVED BY : PONGSAK J.

ISSUED DATE : 27-Jan-25

RECEIVED DATE : 15-Jan-25

THIS CERTIFICATE MAY NOT BE REPRODUCED OTHER THAN IN FULL EXCEPT WITH THE PRIOR WRITTEN APPROVAL OF
QUALITY CALIBRATION CO., LTD.



F-G010 REV : 03

**QUALITY CALIBRATION CO., LTD.**

235 Petchkasem 63/2 Road, Laksong, Bangkai, Bangkok 10160

Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

CERTIFICATE No : 25T0520

PAGE : 2 OF 2

Calibration Report

EQUIPMENT : COD REACTOR

MANUFACTURER : HACH

ID NUMBER : DRB 05/59

RECEIVED DATE : 15-Jan-25

AMBIENT TEMPERATURE : 23°C ± 1°C

MODEL : DRB 200

SERIAL NUMBER : 15110C0497

CALIBRATION DATE : 27-Jan-25

RELATIVE HUMIDITY : 53 %RH ± 10 % RH

CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED BY DIRECT MEASUREMENT METHOD WITH CALIBRATED THERMOCOUPLE TYPE K UNDER NO LOAD CONDITION. THE THERMOCOUPLES WERE PLACED ON POINTS AND LOCATED AS THE PICTURE.


2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) DATA LOGGER WITH TC TYPE K	HYDRA 2635A	6635300	24T6468	26-Jun-25

3. THE CERTIFICATE IS VALID FOR THE ITEM CALIBRATED AS SHOWN ON THE DATE AND PLACE OF CALIBRATION ONLY.

4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.

5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-
- NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH QUALITY CALIBRATION CO., LTD.

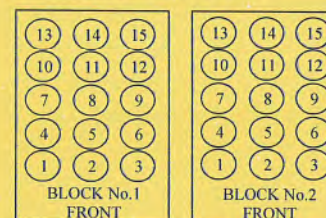RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

Block No.	1	2	
Calibration Point (°C)	150	150	
Controller temperature (°C)	144	144	
Indicating Temperature	144	144	
Measured Temperature (° C) at Spread Locations	1	150.01	149.57
	2	150.69	150.44
	3	150.40	149.46
	4	150.22	149.89
	5	150.27	149.75
	6	150.51	150.45
	7	150.24	150.03
	8	150.20	150.08
	9	150.14	150.14
	10	149.70	149.83
	11	149.58	149.89
	12	149.46	149.79
	13	148.77	149.03
	14	148.99	149.14
	15	149.02	149.62
Uncertainty of Measurement(± °C)	0.87	0.87	

NOTE 1 : THE UNCERTAINTY OF MEASUREMENT EXCLUDED TEMPERATURE UNIFORMITY OF THE CHAMBER.

NOTE 2 : LOCATION 10 WAS REFERENCE LOCATION.

NOTE 3 : THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA.

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR k=2, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT



F-G010 REV : 03



CERTIFICATE No : 25M2256
REFERENCE No : 76365-3

PAGE : 1 OF 2

Certificate of Calibration

EQUIPMENT : DIGITAL BALANCE
MANUFACTURER : SARTORIUS
MODEL : BSA224S-CW
SERIAL No : 36591843
ID No : BA09/61
CONDITION AS RECEIVED : USED ITEM
SUBMITTED BY : S.P.S. CONSULTING SERVICE CO., LTD.
7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN RD.,
JOMPOL, CHATUCHAK, BANGKOK 10900

CALIBRATED BY : ATSAWIN Y.
CALIBRATION DATE : 07-Mar-25

APPROVED BY : PONGSAK J.

ISSUED DATE : 13-Mar-25

RECEIVED DATE : 07-Mar-25

THIS CERTIFICATE MAY NOT BE REPRODUCED OTHER THAN IN FULL EXCEPT WITH THE PRIOR WRITTEN APPROVAL OF
QUALITY CALIBRATION CO., LTD.



CERTIFICATE No : 25M2256

PAGE : 2 OF 2

Calibration Report

EQUIPMENT : DIGITAL BALANCE MODEL : BSA224S-CW
MANUFACTURER : SARTORIUS S/N : 36591843
ID No : BA09/61 RECEIVED DATE : 07-Mar-25
AIR PRESSURE : 1009mbar \pm 1mbar CALIBRATION DATE : 07-Mar-25
AMBIENT TEMPERATURE : 24° C \pm 1° C RELATIVE HUMIDITY : 52 %RH \pm 10 % RH

CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED BY ACCORDING TO UKAS LAB 14 EDITION 6:2019 BY USING KNOWN WEIGHT STANDARD WEIGHT. THE BALANCE WAS NOT ADJUSTED BEFORE CALIBRATION. THE BALANCE HAS NO ZERO TRACKING FUNCTION. REPEATABILITY WAS MEASURED BY USING 10 REPEATED MEASUREMENTS. LINEARITY WAS MEASURED COVERING 10 POINTS, EVENLY SPREAD OVER THE RANGE. THE INSTRUMENT WAS SET ZERO BEFORE PERFORMING THE LINEARITY TEST. OFF-CENTER LOADING WAS MEASURED BY USING STANDARD WEIGHTS PLACED ON THE PAN AND MOVED TO VARIOUS POSITIONS ON THE PAN.

2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) STANDARD WEIGHT SET	E2	QK-I-151	C02250116	28-Jan-27
2) STANDARD WEIGHT	E2	15843	C02250117	29-Jan-27

3. THE CERTIFICATE IS VALID FOR THE ITEM CALIBRATED AS SHOWN ON THE DATE AND PLACE OF CALIBRATION ONLY.

4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.

5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-
- NATIONAL INSTITUTE OF METROLOGY (THAILAND)

RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

- ZERO SETTING FUNCTION : NORMAL
- TARE FUNCTION : NORMAL
- REPEATABILITY OF READING AT 200 g WAS 0.000071 g
- DEPARTURE FROM NOMINAL VALUE/ LINEARITY

NOMINAL VALUE (g)	BALANCE READING (g)	CORRECTION (g)	UNCERTAINTY (\pm g)
0.00	0.0000	0.0000	0.00012
0.10	0.1000	0.0000	0.00012
0.20	0.2000	0.0000	0.00012
0.50	0.5000	0.0000	0.00012
1.00	1.0000	0.0000	0.00012
2.00	2.0000	0.0000	0.00012
5.00	5.0000	0.0000	0.00012
10.00	10.0000	0.0000	0.00012
20.00	20.0001	-0.0001	0.00012
50.00	50.0000	0.0000	0.00014
100.00	100.0001	-0.0001	0.00019
200.00	200.0001	-0.0001	0.00032

5. OFF CENTER LOADING ERROR



POINT	READING (g)
1	100.0000
2	100.0000
3	100.0000
4	100.0000
5	100.0000
OFF-CENTER LOADING	0.0000

NOTE: THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA
THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A
COVERAGE FACTOR $k=2$, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT





บริษัท ไทยยูนิค จำกัด THAI UNIQUE CO., LTD.

80-82 ถนนประชาธิปไตย แขวงบางขุนพรหม เขตพระนคร กรุงเทพฯ 10200

80-82 Prachathipatai Rd., Bangkhunphrom, Pranakorn, Bangkok 10200

Tel. 0-2629-0191-6, 0-2280-1787, Fax. 0-2280-1788, E-mail : thawatt@thaiunique.com, Website : www.thaiunique.com

GAS CHROMATOGRAPH TEST CERTIFICATION

Certificate No. : SV0825/23032

Instrument Type : Gas Chromatography

Model : 3800

Serial Number : 00734

Organization : S.P.S. Consulting Service Co., Ltd.

Address : 7 Phahonyothin Soi 24 Phahonyothin Rd. Ladyao Chatuchak Bangkok 10900

Date : 02/08/2025

ELECTRONIC TEST

CPU	<input checked="" type="checkbox"/> PASS	<input type="checkbox"/> FAIL
DISPLAY & LED TEST	<input checked="" type="checkbox"/> PASS	<input type="checkbox"/> FAIL
VENT TEST	<input checked="" type="checkbox"/> PASS	<input type="checkbox"/> FAIL
KEY ECHO TEST	<input checked="" type="checkbox"/> PASS	<input type="checkbox"/> FAIL
DESTRUCTION RAM TEST	<input checked="" type="checkbox"/> PASS	<input type="checkbox"/> FAIL

RUN CHROMATOGRAM TEST

DETECTOR : Flame Ionization Detectors (FID Channel-Front)

INJECTOR : 1079 Injector

GC CONDITION:

Column	80 °C hold 1 min., rate 20 °C/min. to 200 °C hold 1min.
Injector	220 °C
Detector	300 °C
Column flow	5 mL/min
Makeup flow	25 mL/min
Air flow	300 mL/min
Hydrogen flow	30 mL/min

Column:Capillary Column CP sil 5 CB 0.25 ID x 15 M

Sample: 1 µL Injection FID Test Sample 0.218g/L C14,C15,C16 in hexane (diluted to 30ppm)

SENSITIVITY TEST: C15. (Area count) = 515,940 Counts.



บริษัท ไทยยูนิค จำกัด THAI UNIQUE CO., LTD.

80-82 ถนนประชาธิปไตย แขวงบางขุนพรหม เขตพระนคร กรุงเทพฯ 10200

80-82 Prachathipatai Rd., Bangkhunphrom, Pranakorn, Bangkok 10200

Tel. 0-2629-0191-6, 0-2280-1787, Fax. 0-2280-1788, E-mail : thawatt@thaiunique.com, Website : www.thaiunique.com

Detector Sensitivity (FID)

Detector Response	Result	Specification
Baseline Noise (µV)	2.40	≤ 50
Baseline Drift (%)	0.18	≤ 1
Sensitivity (S/N for C15)	19,716	≥ 1,024


Temperature Specification

Temperature	Set	Result	Specification
Column Oven (°C)	80	79	± 5
Injector (°C)	220	218	± 5
Detector (°C)	300	298	± 5
Incubator (°C)	60	N/A	± 5

Relative Standard Deviation % (%RSD)

Checkout Procedure	Result	Specification
Area C15 (%)	1.48	≤ 5
Retention Time C15 (%)	0.08	≤ 0.5

APPROVAL :

Signature: 

Engineer : Somchai Pohtongkam

Date : 02/08/2025



VARIAN

1/2

SERVICE DEPARTMENT

FR-SV-029 Rev. 04



VARIAN

2/2

SERVICE DEPARTMENT

FR-SV-029 Rev. 04



บริษัท ไทยยูนิค จำกัด

THAI UNIQUE CO., LTD.

80-82 ถนนประชาธิปไตย แขวงบางขุนพรหม เขตพระนคร กรุงเทพฯ 10200

80-82 Prachathipatai Rd., Bangkhunphrom, Pranakorn, Bangkok 10200

Tel. 0-2629-0191-6, 0-2280-1787, Fax. 0-2280-1788, E-mail : thawatt@thaiunique.com, Website : www.thaiunique.com

Results Integrated System Testing

Checkout Procedure	FID
Detector Position	Front
Inlet Type	1079 Injector
C15 Area 1	506,043
C15 Area 2	520,497
C15 Area 3	522,154
C15 Area 4	521,664
C15 Area 5	509,340
C15 Area Average	515,940
* % RSD (< 5 %)	1.48

* The precision specification should be less than 2.0 % RSD ** (Relative Standard Deviation) for an Auto sampler injection and less than 5 % for Manual injections. To calculate the %RSD, select the C15 peak area for each of the five (5) samples.

** (Relative Standard Deviation is determined by dividing the standard deviation by the average and multiplying by 100.)

$$\% \text{ RSD} = (\text{std.dev} / \text{avg}) * 100$$

Compliance	<input checked="" type="checkbox"/> Pass	<input type="checkbox"/> Fail
Performance by	Sankul P.	
Date	02/08/2025	



Comments			
Reviewed by	Wattana	Date	02/08/2025



บริษัท ไทยยูนิค จำกัด

THAI UNIQUE CO., LTD.

80-82 ถนนประชาธิปไตย แขวงบางขุนพรหม เขตพระนคร กรุงเทพฯ 10200

80-82 Prachathipatai Rd., Bangkhunphrom, Pranakorn, Bangkok 10200

Tel. 0-2629-0191-6, 0-2280-1787, Fax. 0-2280-1788, E-mail : thawatt@thaiunique.com, Website : www.thaiunique.com

Results Integrated System Testing

Checkout Procedure	FID
Detector Position	Front
Inlet Type	1079 Injector
C15 RT 1	3.874
C15 RT 2	3.880
C15 RT 3	3.875
C15 RT 4	3.872
C15 RT 5	3.878
C15 RT Average	3.876
* % RSD (< 0.5 %)	0.08

* The precision specification should be less than 0.5 % RSD ** (Relative Standard Deviation) for an Auto sampler injection and less than 0.5 % for Manual injections. To calculate the %RSD, select the RT C15 peak for each of the five (5) samples.

** (Relative Standard Deviation is determined by dividing the standard deviation by the average and multiplying by 100.)

$$\% \text{ RSD} = (\text{std.dev} / \text{avg}) * 100$$

Compliance	<input checked="" type="checkbox"/> Pass	<input type="checkbox"/> Fail
Performance by	Sankul P.	
Date	02/08/2025	



Comments			
Reviewed by	Wattana	Date	02/08/2025



VARIAN

1/1

SERVICE DEPARTMENT



VARIAN

1/1

SERVICE DEPARTMENT


Title :
Run File : e:\sps2025\blk001.run
Method File : c:\star\data\tu\2025\cal fid.mth
Sample ID : blk

Injection Date: 2/8/2568 12:01 Calculation Date: 2/8/2568 12:33

Operator : watsamon Detector Type: 3800 (10 Volts)
Workstation: GC-LAB Bus Address : 44
Instrument : Sample Rate : 10.00 Hz
Channel : Front = FID Run Time : 20.005 min

** LC Workstation Version 6.20 ** 02511-7390-ae7-0265 **

Chart Speed = 1.13 cm/min Attenuation = 1 Zero Offset = 50%
Start Time = 0.000 min End Time = 20.005 min Min / Tick = 1.00

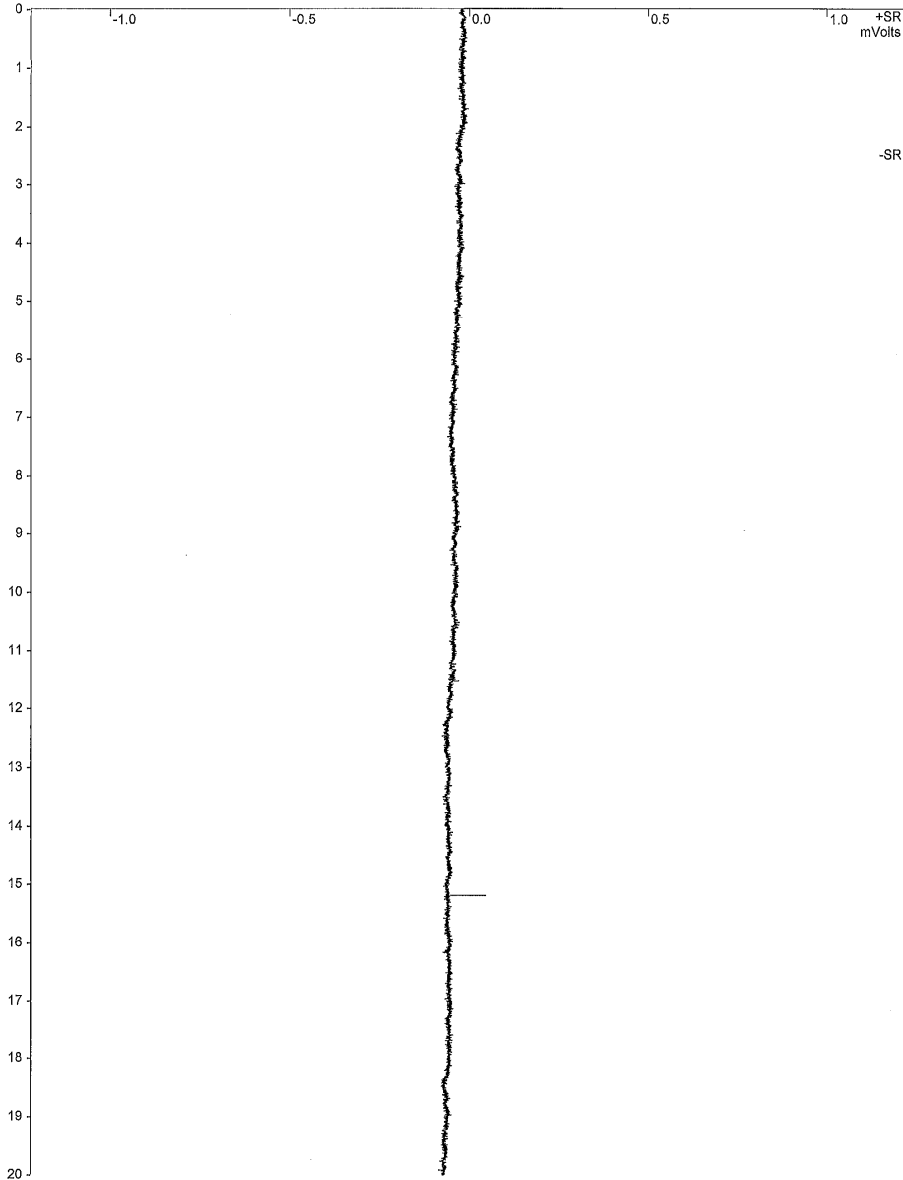

Title :
Run File : e:\sps2025\blk001.run
Method File : c:\star\data\tu\2025\cal fid.mth
Sample ID : blk

Injection Date: 2/8/2568 12:01 Calculation Date: 2/8/2568 12:33

Operator : watsamon Detector Type: 3800 (10 Volts)
Workstation: GC-LAB Bus Address : 44
Instrument : Sample Rate : 10.00 Hz
Channel : Front = FID Run Time : 20.005 min

** LC Workstation Version 6.20 ** 02511-7390-ae7-0265 **

Run Mode : Analysis
Peak Measurement: Peak Area
Calculation Type: External Standard

Peak No.	Peak Name	Result ()	Ret. Time (min)	Time Offset (min)	Area (counts)	Sep. Code	Width 1/2 (sec)	Status Codes
Totals:		0.0000		0.000	0			

Total Unidentified Counts : 0 counts

Detected Peaks: 0 Rejected Peaks: 0 Identified Peaks: 0

Multiplier: 1 Divisor: 1 Unidentified Peak Factor: 0

Baseline Offset: -14 microVolts LSB: 1 microVolts

Noise (used): 24 microVolts - monitored before this run

Manual injection

Data Handling: No peaks


Title :
Run File : e:\sps2025\fidstd001.run
Method File : c:\star\data\tu\2025\cal fid.mth
Sample ID : fidstd

Injection Date: 2/8/2568 12:34 Calculation Date: 2/8/2568 13:26

Operator : watsamon Detector Type: 3800 (10 Volts)
Workstation: GC-LAB Bus Address : 44
Instrument : Sample Rate : 10.00 Hz
Channel : Front = FID Run Time : 7.993 min

** LC Workstation Version 6.20 ** 02511-7390-ae7-0265 **

Chart Speed = 2.83 cm/min Attenuation = 79 Zero Offset = 2%
Start Time = 0.000 min End Time = 7.993 min Min / Tick = 1.00

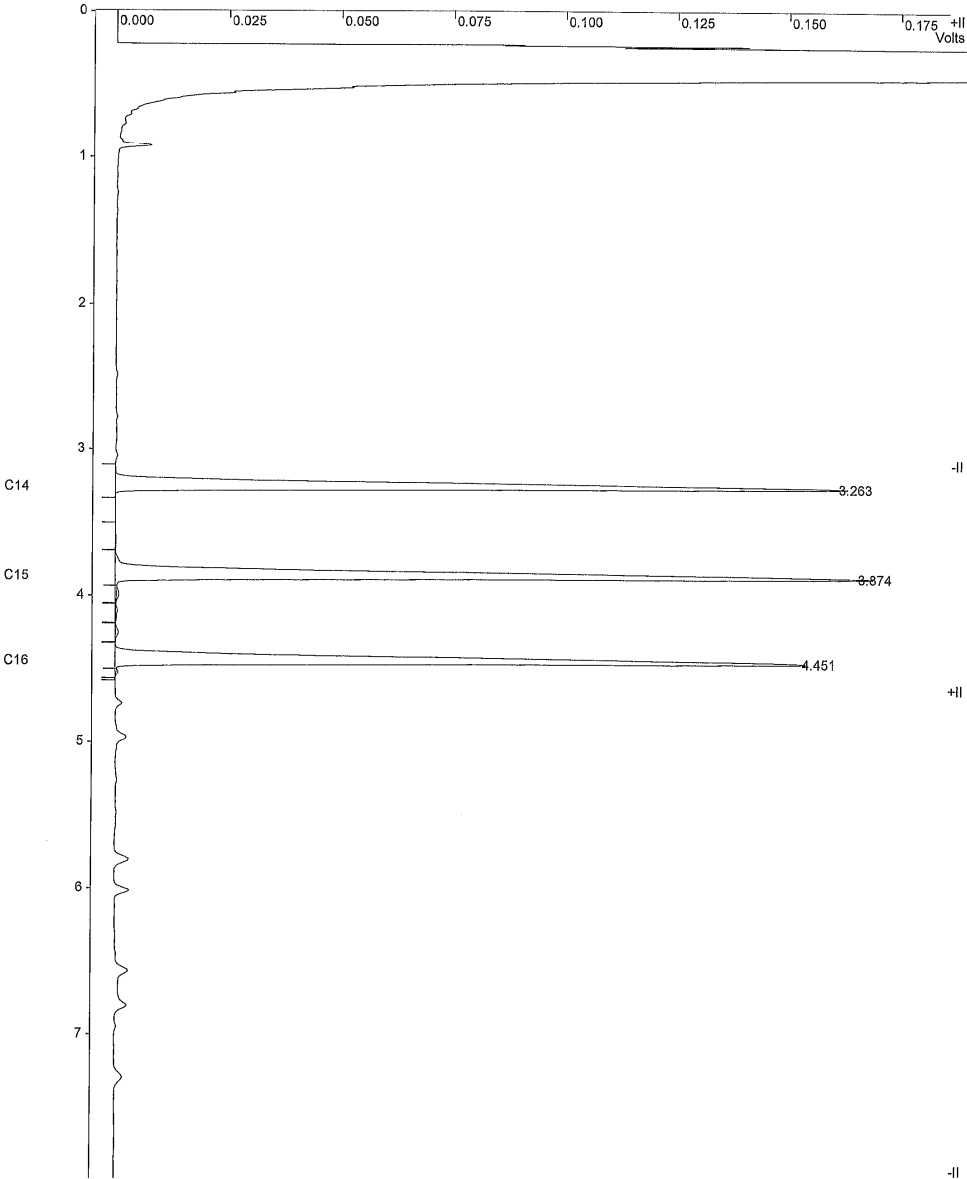

Print Date: Sat Aug 02 15:10:09 2025 Page 1 of 1

Title :
Run File : e:\sps2025\fidstd001.run
Method File : c:\star\data\tu\2025\cal fid.mth
Sample ID : fidstd

Injection Date: 2/8/2568 12:34 Calculation Date: 2/8/2568 13:26

Operator : watsamon Detector Type: 3800 (10 Volts)
Workstation: GC-LAB Bus Address : 44
Instrument : Sample Rate : 10.00 Hz
Channel : Front = FID Run Time : 7.993 min

** LC Workstation Version 6.20 ** 02511-7390-ae7-0265 **

Run Mode : Calibration
Peak Measurement: Peak Area
Calculation Type: External Standard
Level : 1

Peak No.	Peak Name	Ret. Time (min)	Time Offset (min)	Area (counts)	Sep. Code	Width 1/2 (sec)	Status Codes
1	C14	3.263	0.002	458627	BB	2.7	
2	C15	3.874	0.002	506043	VV	2.8	
3	C16	4.451	0.001	460610	VB	2.8	
Totals:			0.005	1425280			

Total Unidentified Counts : 0 counts

Detected Peaks: 8 Rejected Peaks: 5 Identified Peaks: 3

Multiplier: N/A Divisor: N/A Unidentified Peak Factor: 0

Baseline Offset: 6 microVolts LSB: 1 microVolts

Noise (used): 2 microVolts - monitored before this run

Manual injection

Sample ID: fid std


Operator (Inj): watsamon
Injection Date: 02/08/2025
Calc Date: 02/08/2025
Run Time (min): 7.993
Workstation: GC-LAB
Instrument (Inj):

**VARIAN**

Run Mode: Calibration
Peak Measurement: Peak Area
Calculation Type: External Std.

e:\sps2025\fidstd001.run

A = FID 10 V RESULTS

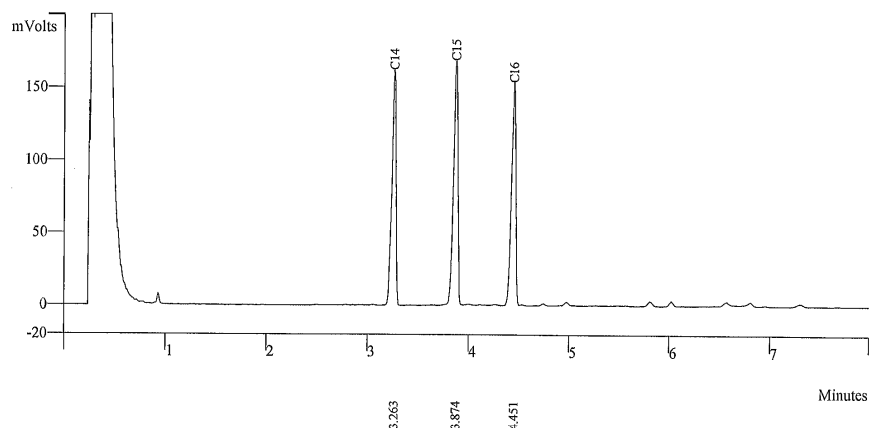

Peak No	Peak Name	Result ()	Ret Time (min)	Peak Area (counts)	Sep. Code	Width 1/2 (sec)
1	C14	0.0000	3.263	458627	BB	2.7
2	C15	0.0000	3.874	506043	VV	2.8
3	C16	0.0000	4.451	460610	VB	2.8
Totals		0.0000		1425280		



Sample ID: fid std


Operator (Inj): watsamon
Injection Date: 02/08/2025
Calc Date: 02/08/2025
Run Time (min): 7.993
Workstation: GC-LAB
Instrument (Inj):

**VARIAN**

Run Mode: Calibration
Peak Measurement: Peak Area
Calculation Type: External Std.

e:\sps2025\fidstd002.run

A = FID 10 V RESULTS

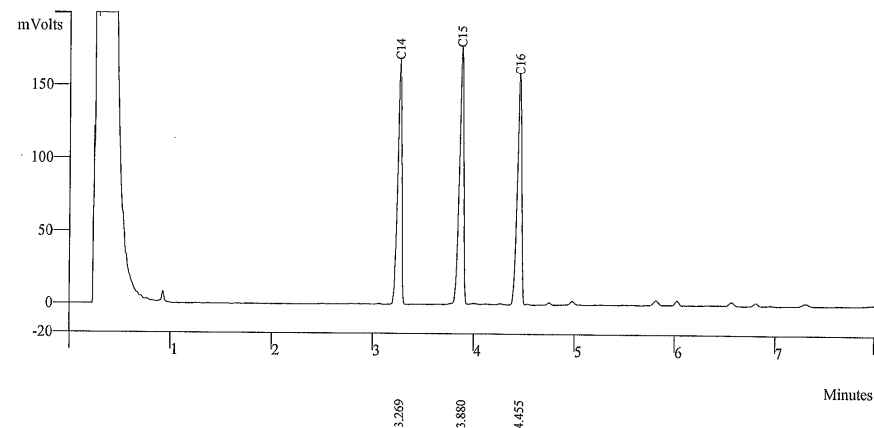

Peak No	Peak Name	Result ()	Ret Time (min)	Peak Area (counts)	Sep. Code	Width 1/2 (sec)
1	C14	0.0000	3.269	472338	BB	2.6
2	C15	0.0000	3.880	520497	VV	2.7
3	C16	0.0000	4.455	471916	VB	2.8
Totals		0.0000		1464751		



Sample ID: fid std

Operator (Inj): watsamon

Injection Date: 02/08/2025

Calc Date: 02/08/2025

Run Time (min): 7.993

Workstation: GC-LAB

Instrument (Inj):

**VARIAN**


Run Mode: Calibration

Peak Measurement: Peak Area

Calculation Type: External Std.

e:\sps2025\fidstd003.run

A = FID 10 V RESULTS

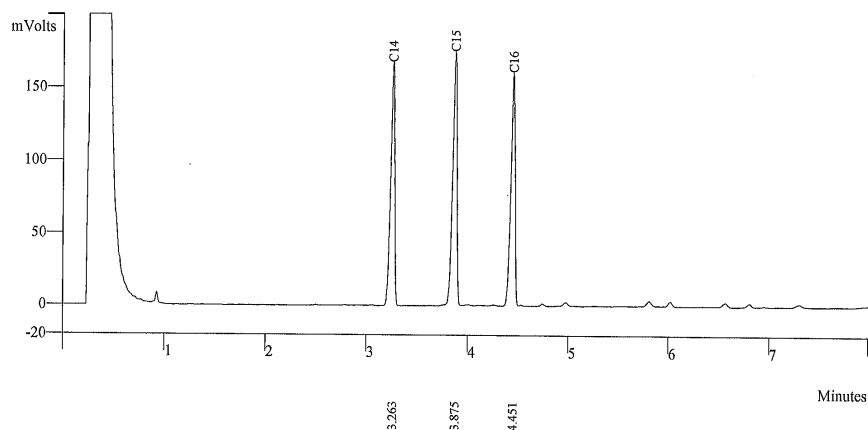

Peak No	Peak Name	Result ()	Ret Time (min)	Peak Area (counts)	Sep. Code	Width 1/2 (sec)
1	C14	0.0000	3.263	469265	BB	2.6
2	C15	0.0000	3.875	522154	VV	2.8
3	C16	0.0000	4.451	478526	VB	2.8
Totals		0.0000		1469945		



Sample ID: fid std

Operator (Inj): watsamon

Injection Date: 02/08/2025

Calc Date: 02/08/2025

Run Time (min): 7.993

Workstation: GC-LAB

Instrument (Inj):

**VARIAN**


Run Mode: Calibration

Peak Measurement: Peak Area

Calculation Type: External Std.

e:\sps2025\fidstd004.run

A = FID 10 V RESULTS

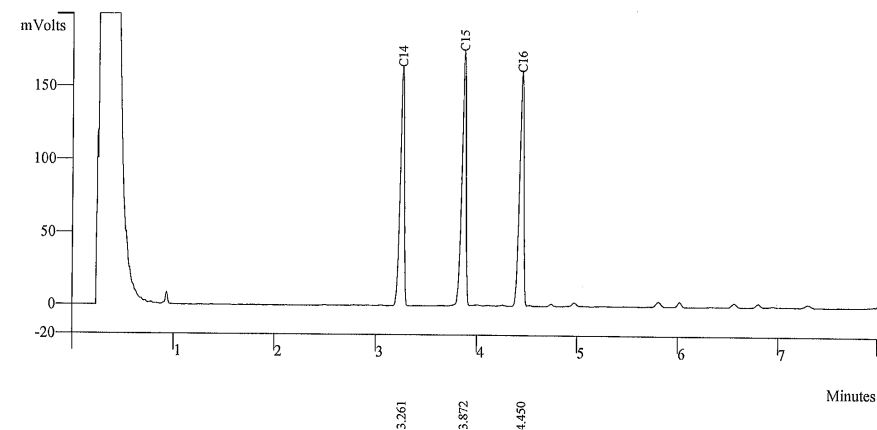

Peak No	Peak Name	Result ()	Ret Time (min)	Peak Area (counts)	Sep. Code	Width 1/2 (sec)
1	C14	0.0000	3.261	468907	BB	2.7
2	C15	0.0000	3.872	521664	VV	2.8
3	C16	0.0000	4.450	478772	VB	2.8
Totals		0.0000		1469343		



Sample ID: **fid std**


Operator (Inj): watsamon
Injection Date: 02/08/2025
Calc Date: 02/08/2025
Run Time (min): 7.993
Workstation: GC-LAB
Instrument (Inj):



Run Mode: Calibration
Peak Measurement: Peak Area
Calculation Type: External Std.

e:\sps2025\fidstd005.run

A = FID 10 V RESULTS

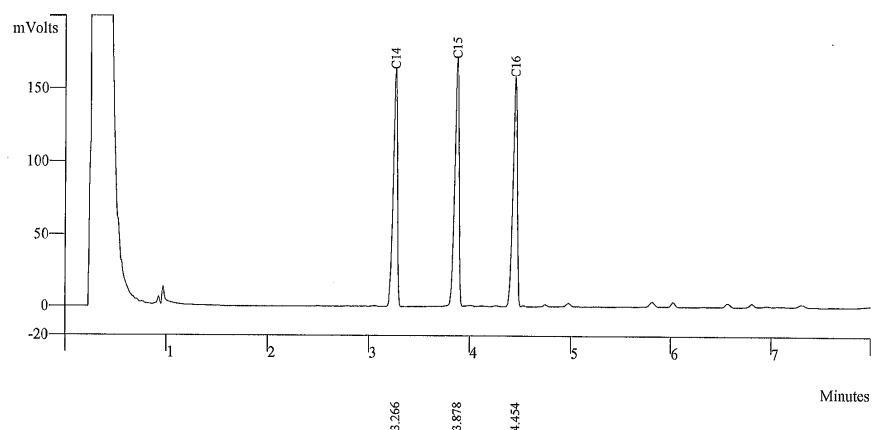

Peak No	Peak Name	Result ()	Ret Time (min)	Peak Area (counts)	Sep. Code	Width 1/2 (sec)
1	C14	0.0000	3.266	459351	BB	2.6
2	C15	0.0000	3.878	509340	VV	2.8
3	C16	0.0000	4.454	468353	VB	2.8
Totals		0.0000		1437044		



THAI UNIQUE CO.,LTD.


1 Of 1

Print Date: 02 Aug 2025 15:12:58
Calibration Curves Report
File: e:\sps2025\cal fid.mth
Detector: 3800 GC, Address: 44, Channel ID: Front

C14

External Standard Analysis
Curve Type: Linear
Origin: Force
 $y = +1.552325e+004x$


Resp. Fact. RSD: 1.347%
Coeff. Det.(r²): 0.999130

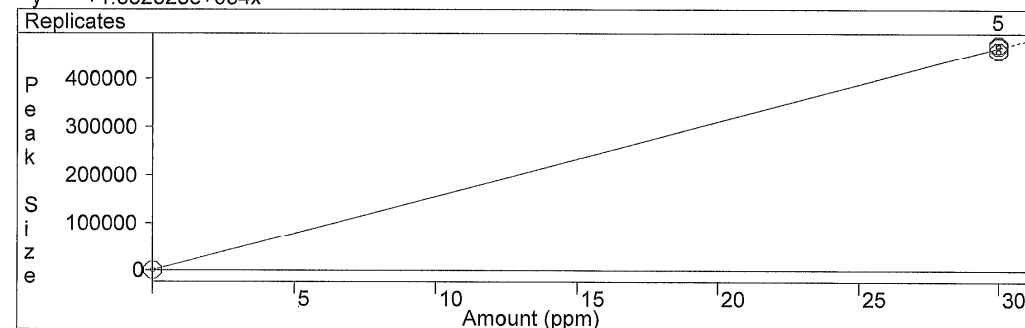

C15

External Standard Analysis
Curve Type: Linear
Origin: Force
 $y = +1.719798e+004x$


Resp. Fact. RSD: 1.481%
Coeff. Det.(r²): 0.998948

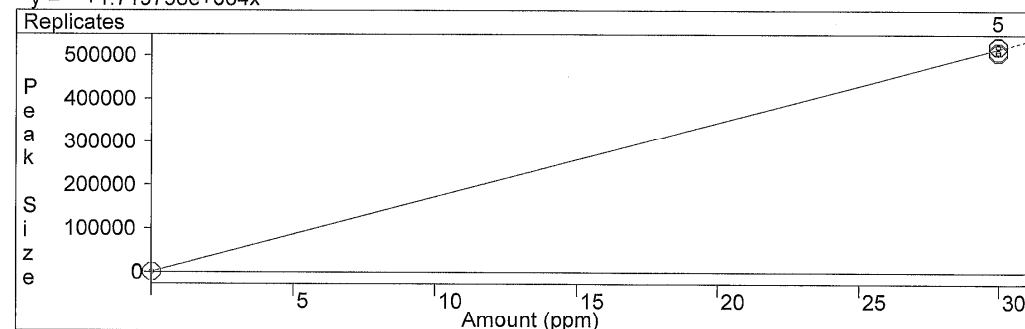

C16

External Standard Analysis
Curve Type: Linear
Origin: Force
 $y = +1.572118e+004x$

Resp. Fact. RSD: 1.611%
Coeff. Det.(r²): 0.998756

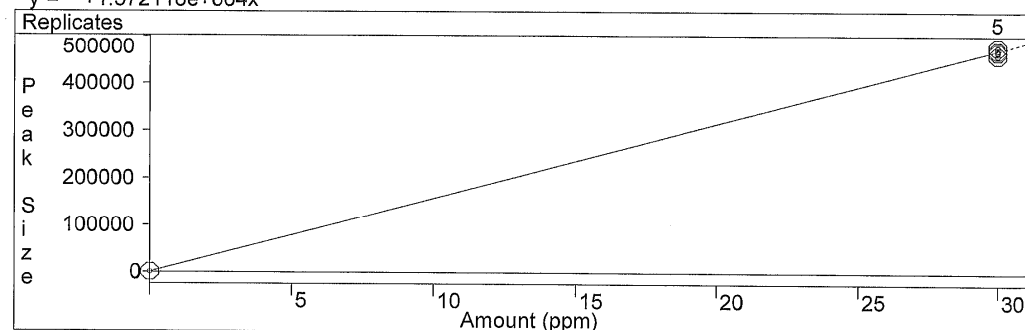

CERTIFICATE

This is to certify, that

Somchai Pohthongkham

has participated the course

Basic GC and Sampler training

Date: **24 – 27 May 2004**

Location: **Middelburg**

Instructor: **W.J. Buys**

Signature instructor: 



Varian Analytical Instruments
Varian Chrompack International BV
Herculesweg 8
P.O. Box 8033
4330 EA Middelburg
The Netherlands
Tel.: +31 118 671000
Fax: +31 118 631118
www.varianinc.com



WK Electric Co., Ltd.

68/242 Moo 5, Sawalpracharaj Rd., Tumbol Ladsawai, Amphur Lamlukka, Pathumthani 12150

Tel. +66 2993 4773, +66 2153 7132-3 Fax. +66 2994 5509 E-mail : wk.calibrations@gmail.com www.wk-etc.com



Certificate of Calibration

Certificate No.: WK2412-053-1

Page 1 of 2

Customer : THAI UNIQUE CO., LTD.
80-82 Prachathipatai Rd., Bangkokphrom,
Pranakorn, Bangkok 10200

Instrument	: AMD Flow Meter	Ambient Temperature	: (23 ± 2) °C
Manufacturer	: Agilent Technologies	Humidity	: (50 ± 15) %RH
Model	: G6691A	Received Date	: 4-Dec-24
Serial No.	: MY16470347	Calibrated Date	: 11-Dec-24
Identity No.	: SV-DF-001	Issued Date	: 13-Dec-24
Range	: 0 ml/min to 750 ml/min	Calibrated Location	: In Lab
Resolution	: See to Data		
Calibration Method	: CP-WK-M10		

Reference standard instruments :

Instrument	Serial No.	Certificate No.	Due Date	Traceability to
Flow Calibrator	140215-134	L202304114-001	18-Apr-25	MIT
Primary Flow Calibrator	1107-S	WK2405-049-5	22-May-25	WK Electric Co., Ltd.


MIT : Miracle International Technology Co., Ltd.

This result calibrate was found accurate as shown on date place of calibrate only
This certificate is traceability to the International System of Unit (SI)

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k=2$, providing a level of confidence approximately 95%

Calibrated by : Mr.Thippatai Mungpungklang

Approved by :


Ms. Budsagorn Patcha

Authorized Signatory

This certificate may not be reproduced except in full unless permission for the reproduction has been obtained in writing from the laboratory.



Measuretronix Limited
2425/2 Lat Phrao Road, Saphan Song
Wangthonglang, Bangkok 10310, Thailand
Phone : 0-2514-1000, 0-2514-1234
Fax : 0-2514-0001, 0-2514-0003
Website : www.measuretronix.com



Certificate of Calibration

Certificate Number : LF25-0305
Equipment : Thermometer
Manufacturer : Fluke
Model : 51
Serial Number : 5910857
Asset Number : 5910857
Customer : Thai Unique Co., Ltd.
80-82 Prachathipatai Road,
Bangkhunphrom, Pranakorn,
Bangkok 10200
Date of Calibrate : 6-Jun-2025
Date of Issue : 6-Jun-2025

This calibration certificate documents the traceability to national standards, which realize the units of measurement according to the International System of Units (SI).

This calibration certificate applies only to the item identified and shall not be reproduced other than in full, without specific written approval by Measuretronix Cal-Lab. Calibration certificates without signature are not valid.

The measurements marked with an asterisk () in this certificate are outside our range of accreditation. They have been included for completeness.*

The Calibration interval (Cal.Due) is the responsibility of the end user.

Calibrated by

Samak

Mr. Samak Uaonkaonoi
Metrology Technician

Approved by

Miss Juthamas Sukhathairun

Miss Juthamas Sukhathairun
Cal-Lab Manager



Agilent Technologies

Certificate of Analysis

FID-TCO Performance Evaluation Sample Kit

Agilent Part Number: 5080-8842, 18710-60170

Sample Lot Number: 0006750304

This analytical reference material was manufactured and verified in accordance with an ISO 9001 registered quality system, and the analyte concentrations were verified by an ISO 17025 accredited laboratory. The certified value for each analyte was determined gravimetrically.

Concentrations:		
n-tetradecane	0.218 g/L ($\pm 0.5\%$)	0.033 w/w %
n-pentadecane	0.218 g/L ($\pm 0.5\%$)	0.033 w/w %
n-hexadecane	0.218 g/L ($\pm 0.5\%$)	0.033 w/w %


Solvent: hexane

Calibrated Class A glassware and clean bottles were used in the manufacture of this standard. Balances used in the manufacture of this standard are calibrated with weights traceable to NIST in compliance with ANSI/NCCL Z-540-1 and ISO 9001.

Purities:	
n-tetradecane	99.6%
n-pentadecane	99%
n-hexadecane	99.5%
hexane	99%

Typical Analytical Spectrum or Chromatography

GC Chromatography – n-tetradecane, n-pentadecane, and n-hexadecane in hexane

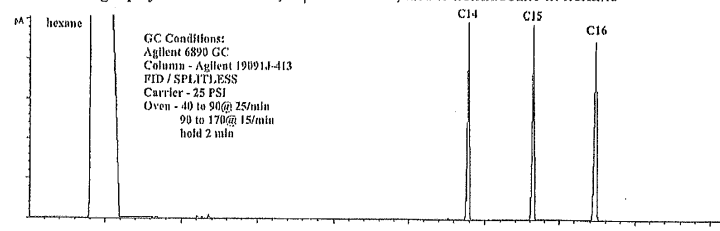


Date of release: 30 June 2023

Date of expiration: 31 July 2025

Monica Bourgeois
Monica Bourgeois
QMS Representative

GC Clarus 600/680 Preventive Maintenance (PM)

Company Name:	S.P.S. Consulting Service Co.,Ltd		
Address (Instrument Location):	7 Soi Phaholyothin24 Phaholyothin Road, Jompol, Chatuchak, Bangkok, 10900.		
Serial Number:	680S14042502	Service Tag:	N68APSSFEMP
Customer Name (if applicable):	Ms.Naruecha	PM number :	2 of 2
Service Engineer Name:	Monchai Kitcharoenkeat	Service Order Number:	WO-06815714
Date PM Performed: (DD-MMM-YYYY)	13-Aug-2025	Next PM Due Date: (DD-MMM-YYYY)	13-Feb-2026

Part Number	Release	Publication Date	
TH09370070	C	August 2016	

Scope

The purpose of this PM is to ensure the continued functionality of the Clarus 600 and Clarus 680 GC by inspecting and replacing any worn or damaged parts. This service should only be performed by a trained representative of PerkinElmer. The customer should save their method before the PM begins.

General Instructions:

The customer must provide the engineer operational data to demonstrate recent instrument performance prior to starting the PM. Always check with the customer before making any changes that may affect the customer's analysis or calibration, including a current back-up of system software and/or data files. The completed document should be signed by an authorized PerkinElmer and customer representative and left with the customer. Update the PM sticker and instrument logbook as required.

Copyright Information

This document contains proprietary information that is protected by copyright. All rights are reserved. No part of this publication may be reproduced in any form whatsoever or translated into any language without the prior, written permission of Perkin Elmer, Inc. Copyright © 2013 PerkinElmer, Inc.

Trademarks

Registered names, trademarks, etc. used in this document, even when not specifically marked as such, are protected by law. PerkinElmer is a registered trademark of PerkinElmer, Inc. All other trademarks and registered trademarks not owned by PerkinElmer, Inc. or its subsidiaries that are depicted herein are the property of their respective owners. **Except as specifically set forth in its terms and conditions of sale, PerkinElmer makes no Warranty of any kind with regard to this document, including, but not limited to, the implied warranties of merchantability and fitness for a particular purpose.** PerkinElmer shall not be liable for incidental or consequential damages in connection with the furnishing or use of this document.

Component List

Component / Specific Model	Serial #	Software Version	Configuration Notes
Clarus680	680S14042502	Totalchrom6.3.2	PSS, PSS, FID,
Clarus SQ8T	648N4050804	Turbomass 6.4	
AtomX	US14113002	Tekma AtomX	

Parts Lists

Additional Tools Required for PM				
Part Number (if applicable)	Description	Quantity	Serial #	Calibration Due Date (MM/YY)
N/A				
Additional Reagents and Standards Required for PM				
Part Number (if applicable)	Description	Quantity	Batch/Lot #	Expiration Date (MM/YY)
N/A				

Procedure Checklist

Use (✓) to check off those steps in the checklist that have been completed.

1. General:

- ☒ Review the instrument performance with the customer and document any recent problems.
- ☒ Check incoming AC line voltage for proper levels and grounding.
 L-N 220 Volt
 L-G 220 Volt
 N-G 0.32 Volt

**Neutral to ground not more than 0.5 volts peak to peak*
- ☒ Inspect all gas line filters and traps; Replace if necessary with customer supplied spares.
 Carrier gas ☒ Helium ☐ Nitrogen ☐ Hydrogen
 Moisture level ☒ Good ☐ Need to replace ☐ Other _____

 Detector gas ☒ Air Zero ☒ Hydrogen ☐ Nitrogen ☐ Helium
 Moisture level ☒ Good ☐ Need to replace ☐ Other _____
- ☒ Inspect the customer log book and make any appropriate PM entries.
- ☒ Leak check all fittings from the gas source to instrument.
 Gas leakage ☒ Pass ☐ Fail Comment _____
- ☒ Perform general inspection of system for cleanliness.
- ☒ Inspect for functional and clean electronic cooling and oven vent fans
 Electronic cooling fan ☒ Yes ☐ No
 Oven cooling fan ☒ Yes ☐ No

2. Electronic :

- ☒ Check oven temperature. Calibrate if necessary.
 Oven temperature set point 150 °C ☒ Pass ☐ Fail
- ☐ Check sub-ambient option. (If installed).
 Oven temperature set point 5 °C ☐ Pass ☐ Fail
- ☒ Perform routine maintenance on detector/injector. Replace parts as necessary with customer supplied spares.

- ☒ Check flows, including split flows if applicable. Calibrate if necessary.
 Carrier flow Pass
 Split flow Pass
- ☒ Check detector gas flows and adjust if necessary.
 Detector flow Pass
- ☒ Autosampler installed ☒ Yes ☐ No
 Check autosampler sensor for wear and replace if necessary.
 Vial sensor Pass
 Door sensor Pass
 Tower sensor Pass
 Plunger sensor Pass
 Elevator sensor Pass
- ☒ Remove syringe, manually flush. Replace with customer supplied spare if necessary.
- ☒ Check firmware version. Upgrade to current levels if necessary.
 Firmware version 6.5
- ☒ Measure all accessible power supply voltages.
 5 Volt Pass
 +15 Volt Pass
 -15 Volt Pass
 24 Volt Pass
- ☒ Record all detector voltage signal.
 Detector Channel A 0.98 mV.
 Detector Channel B NA mV.

3. Diagnostics Tests:

- ☒ Run instrument diagnostics.
 BRAM Pass
 EPROM Pass
- ☒ Run Autosampler diagnostics.
 BRAM Pass
 EPROM Pass

4. Review:

- ☒ Review with the customer PM work performed.
- ☒ Review with the customer routine maintenance procedures.
- ☒ Discuss recommended customer-supplied materials to have on hand
- ☒ Attach PM sticker.
- ☒ Update Logbook.

Additional Comments

Additional Comments Regarding the PM

Review

<i>The preventive maintenance checks and if applicable performance tests for Clarus600/680 GC have been completed.</i>	
<i>This Clarus600/680 GC Pass the preventive maintenance.</i>	
Review of Preventive Maintenance:	
Authorized PerkinElmer Representative: Monchai Kitcharoenkeat <i>Monchai</i>	Date: 13-Aug-2025 (DD-MMM-YYYY)
Authorized Customer Representative: Ms.Naruecha <i>Naruecha</i>	Date: 13-Aug-2025 (DD-MMM-YYYY)

Cert. No. : SP25026
Pages : 1 of 4

Calibration Certificate

Equipment : UV-VIS SPECTROPHOTOMETER
Manufacturer : PERKINELMER
Model : LAMBDA 25
Serial No.: 501S14123010
ID No.: SP03/58
Calibration Mode : WAVELENGTH ACCURACY
PHOTOMETRIC ACCURACY
STRAY LIGHT

Condition As Found : GOOD

Customer : S.P.S CONSULTING SERVICE CO., LTD.
7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN ROAD,
CHOMPHON SUB-DISTRICT, CHATUCHAK DISTRICT,
BANGKOK PROVINCE 10900 THAILAND.

Location : ORGANIC LABORATORY IV

Ambient Temperature : (22.9 ± 5) °C

Relative Humidity : (53.7 ± 25) %

Received Date : 22 AUGUST 2025

Calibration Date : 22 AUGUST 2025

Date of Issue : 25 AUGUST 2025

Calibrated by : Nitinun Srihawan

Approved by : *Wichok B.*
(Wichok Ekpongpradit)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

Cert. No. : SP25026
Job No. : VC68SP0019
Pages : 2 of 4

Calibration Method :

This instrument was calibrated by using on-site calibration procedure In-house method : CP-SP-01
The calibration procedure to direct measurement wavelength accuracy by using wavelength standard solution, Photometric accuracy by using absorbance standard filter and absorbance standard solution
The calibration procedure used was based on ASTM E275-01, ASTM E925-02

Condition of this result of calibration :

1. Certified reference materials

Material	Ref. type	Cell serial No.	Cert. No.	Due Date
Holmium liquid	RM-HL	29706	126461	24/10/2026
Didymium liquid	RM-DL	28912	126462	24/10/2026
Neutral density filter	RM-1N2N3N	13877	126457	24/10/2026
Potassium dichromate solutions	RM-0204060810	14204	126497	25/10/2026
Potassium Iodide solution	-	KI-0701-001	CI-0185-24	14/05/2026

2. This result of calibration was found accurate as shown on date and place of calibration only.

3. This certificate is traceable to the international system of unit maintained at :

3.1 The UK National Physical Laboratory (NPL)

Result of calibration : Wavelength Accuracy

(Without adjustment)

Material	Certified Values of Reference Material (nm)	UUC* Reading (nm)	Error (nm)	Uncertainty ± (nm)	k Factor
RM-HL	278.13	278.21	0.08	0.16	2.00
	361.25	361.39	0.14	0.16	2.00
	467.82	467.71	-0.11	0.16	2.00
	536.56	536.50	-0.06	0.16	2.00
	640.50	640.36	-0.14	0.16	2.00
RM-DL	740.09	739.85	-0.24	0.16	2.00
	864.94	865.12	0.18	0.16	2.00

UUC* = Unit Under Calibration

Cert. No. : SP25026
Job No. : VC68SP0019
Pages : 3 of 4

Result of calibration : Photometric Accuracy

Material	Wavelength (nm)	Filter S/N	Nominal Absorbance (A)	Certified Absorbance (A)	UUC* Reading Absorbance (A)	Error (A)	Uncertainty ± (A)	k Factor
Neutral Density glass filter	440.0	29381	0.5	0.5443	0.5413	-0.0030	0.0043	2.00
		29914	0.7	0.7484	0.7455	-0.0029	0.0054	2.00
		29360	1.0	1.0527	1.0535	0.0008	0.0032	2.00
	465.0	29381	0.5	0.4948	0.4922	-0.0026	0.0041	2.00
		29914	0.7	0.6906	0.6877	-0.0029	0.0050	2.00
		29360	1.0	0.9695	0.9709	0.0014	0.0031	2.00
	546.1	29381	0.5	0.5090	0.5068	-0.0022	0.0036	2.00
		29914	0.7	0.6985	0.6960	-0.0025	0.0041	2.00
		29360	1.0	0.9814	0.9825	0.0011	0.0031	2.00
	590.0	29381	0.5	0.5375	0.5353	-0.0022	0.0034	2.00
		29914	0.7	0.7256	0.7231	-0.0025	0.0037	2.00
		29360	1.0	1.0213	1.0219	0.0006	0.0032	2.00
	635.0	29381	0.5	0.5223	0.5202	-0.0021	0.0033	2.00
		29914	0.7	0.6927	0.6901	-0.0026	0.0036	2.00
		29360	1.0	0.9744	0.9750	0.0006	0.0032	2.00

UUC* = Unit Under Calibration

Cert. No. : SP25026
Job No. : VC68SP0019
Pages : 4 of 4

Result of calibration : Photometric Accuracy

(Without adjustment)

Material	Wavelength (nm)	Solution (mg/l)	Certified Absorbance (A)	UUC* Reading Absorbance (A)	Error (A)	Uncertainty ± (A)	k Factor
Potassium dichromate solutions	235.0	20	0.2415	0.2443	0.0028	0.0101	2.00
		40	0.4866	0.4871	0.0005	0.0115	2.00
		60	0.7415	0.7295	-0.0120	0.0067	2.00
		80	0.9854	0.9844	-0.0010	0.0071	2.00
		100	1.2444	1.2425	-0.0019	0.0073	2.00

UUC* = Unit Under Calibration

Condition of this result of calibration : Spectrophotometer PERKINELMER Model LAMBDA 25 S/N 501S14123010

Resolution of Wavelength Mode 0.1 nm
Resolution of Photometric Mode 0.001 A
Parameter Setting
Measurement Mode Wavelength, Absorbance
Wavelength Scan 190 nm - 1100 nm
Scanning Speed 7.5 nm/min
Band width(Wavelength) 1.0
Band width(Vis) 1.0
Band width(Uv) 1.0

Stray Light** UUC* Reading at 220.0 nm	
Transimission T(%)	Absorbance(A)
0.020	3.7032

**Specific Acceptance :
Transmission ≤ 1.0 T(%), Absorbance ≥ 2.0 A
**Stray light not TISI Accredited

The reported uncertainty is based on a standard uncertainty multiplied by a coverage factor k , providing a level of confidence of approximately 95%

End of Calibration Certificate



WO-11540198/2025

MAINTENANCE AND TEST CERTIFICATE MODEL
OPTIMA 5300DV

Customer : <u>S.P.S.Consulting Service Co.,Ltd</u>	Date Tested: <u>July 1, 2025</u>
Address : <u>7 Soi Phaholyothin 24</u>	Recommendation Recertification
<u>Paholyothin Road</u>	Period <u>6</u> Months
<u>Jompol Chatuchak, Bangkok 1090</u>	Recertification Due: <u>January 1, 2026</u>
User Name: <u>K.Phenpha Viphashtawat</u>	Date Last Certified: <u>January 6, 2025</u>
Phone: <u>083-9269252</u>	Visit Number: <u>1 of 2</u>
Fax: <u>02-513-4221</u>	PerkinElmer Phone: <u>02-719-6420 ext 206</u>
	PerkinElmer Fax: <u>02-318-5597</u>

CONFIGURATION TESTED		ACCESSORIES/COMPONENT NOT INCLUDED
MODEL	SERIAL NUMBER	
<u>OPTIMA 5300DV</u>	<u>077C7042401</u>	
TESTED EQUIPMENT	CALIBRATION NUMBER	EXPIRATION
<u>IPV Methods</u>		
TEST STANDARD USED	PART NUMBER	EXPIRATION DATE
<u>Multielement Standard</u>	<u>N069-1579</u>	<u>December 30, 2024</u>
<u>Wavecal Solution</u>	<u>N058-2152</u>	<u>March 30, 2024</u>
<u>VIS Wavecal solution</u>	<u>N930-2946</u>	<u>February 28, 2024</u>
<u>Instrument Cal. STD4</u>	<u>N930-0221</u>	<u>November 30, 2024</u>
CUSTOMER SUPPLIED	COMMENTS	CUSTOMER INITIALS
<u>2 % HNO3</u>		
<u>10 % HNO3</u>		

Page 1 of 4



WO-11540198/2025

MAINTENANCE AND TEST CERTIFICATE MODEL
OPTIMA 5300DV

SERIAL NUMBER <u>077C7042401</u>	DATE TESTED <u>July 1, 2025</u>
---	--

- MECHANICAL CHECKS**
 - A. Inspect and clean all fans and filters. ☐
 - B. Inspect and replace as necessary, all torch components including the RF coil. ☐
 - C. Inspect all tubing for sign of clacking or leaking. ☐
 - D. Adjust water and gas pressure regulator settings. ☐
 - E. Inspect and leak check pneumatics drawers. ☐
 - F. Clean the exterior of the instrument. ☐
- OPTICAL CHECKS**
 - A. Inspect and clean all optical components. ☐
 - B. As required, check and replace all purgefilters. ☐
 - C. Recheck optical alignment. ☐
- COOLING SYSTEM CHECKS**
 - A. Perform preventive maintenance on chiller. ☐
 - B. Flush out the chiller every year. ☐
- PERFORMANCE CHECKS**
 - A. Torch View Alignment. ☐
 - B. Wavelength Calibration. ☐

Page 2 of 4



MAINTENANCE AND TEST CERTIFICATE MODEL OPTIMA 5300DV

SERIAL NUMBER : 077C7042401		DATE TESTED : July 1, 2025	
PARAMETER	SPECIFICATION	FINAL VALUE	
Spectral Resolution : UV	As 193.696 nm	≤ 0.007	0.00570
	Ni 231.604 nm	≤ 0.008	0.00734
	Ni 341.476 nm	≤ 0.012	0.00763
Spectral Resolution : VIS	La 408.672 nm	≤ 0.020	0.01627
	Ba 455.403 nm	≤ 0.025	0.02428
Precision	As 193.656 nm	% RSD < 1.0	0.82 %
	Zn 213.856 nm	% RSD < 1.0	0.83 %
	Mn 257.610 nm	% RSD < 1.0	0.20 %
	La 379.478 nm	% RSD < 1.0	0.89 %
	Ba 455.403 nm	% RSD < 1.0	0.92 %
	Ba 493.408 nm	% RSD < 1.0	0.75 %
Detection Limits : Axial	Tl 190.080 nm	3(sd)	10.65 ppb
	As 193.696 nm	3(sd)	2.48 ppb
	Pb 220.353 nm	3(sd)	3.09 ppb
Detection Limits : Radial	As 193.696 nm	3(sd)	331.50 ppb
	Zn 213.856 nm	3(sd)	0.98 ppb
	Mn 257.610 nm	3(sd)	0.34 ppb
	La 379.478 nm	3(sd)	2.54 ppb
	Ba 455.403 nm	3(sd)	2.19 ppb
	Ba 493.408 nm	3(sd)	4.32 ppb
BEC : Axial (IB X 500)/(IS-IB)	Cd 226.502 nm	≤ 150 ppb	140.03
BEC : Radial (IB X 1000)/(IS-IB)	Mn 257.610 nm	≤ 45 ppb	24.17



MAINTENANCE AND TEST CERTIFICATE MODEL OPTIMA 5300DV


SERIAL NUMBER	077C7042401	DATE TESTED	July 1, 2025
Remarks :			
Commissioning follow as commissioning performance sheets.			
This is to certify that the above tests have been performed and the configuration tested			
<input checked="" type="checkbox"/> meets			
<input type="checkbox"/> does not meet			
the PerkinElmer Specifications listed on this certificate.			
This certificate does not modify PerkinElmer's standard terms and condition of sale, including warranty terms.			
Service Department-PerkinElmer Ltd.			
Authorized Representative: <u>Wiphan Promlumda</u>			
(Wiphan Promlumda)			
Service Engineer			

เอกสารแนบ 5-5

เอกสารสอบเทียบเครื่องมือการตรวจวิเคราะห์คุณภาพน้ำใต้ดิน

GC Clarus 600/680 Preventive Maintenance (PM)

Company Name:	S.P.S. Consulting Service Co.,Ltd		
Address (Instrument Location):	7 Soi Phaholyothin24 Phaholyothin Road, Jompol, Chatuchak, Bangkok, 10900.		
Serial Number:	680S14042502	Service Tag:	N68APSSFEMP
Customer Name (if applicable):	Ms.Naruecha	PM number :	2 of 2
Service Engineer Name:	Monchai Kitcharoenkeat	Service Order Number:	WO-06815714
Date PM Performed: (DD-MMM-YYYY)	13-Aug-2025	Next PM Due Date: (DD-MMM-YYYY)	13-Feb-2026

Part Number	Release	Publication Date	
TH09370070	C	August 2016	

Scope

The purpose of this PM is to ensure the continued functionality of the Clarus 600 and Clarus 680 GC by inspecting and replacing any worn or damaged parts. This service should only be performed by a trained representative of PerkinElmer. The customer should save their method before the PM begins.

General Instructions:

The customer must provide the engineer operational data to demonstrate recent instrument performance prior to starting the PM. Always check with the customer before making any changes that may affect the customer's analysis or calibration, including a current back-up of system software and/or data files. The completed document should be signed by an authorized PerkinElmer and customer representative and left with the customer. Update the PM sticker and instrument logbook as required.

Copyright Information

This document contains proprietary information that is protected by copyright. All rights are reserved. No part of this publication may be reproduced in any form whatsoever or translated into any language without the prior, written permission of Perkin Elmer, Inc. Copyright © 2013 PerkinElmer, Inc.

Trademarks

Registered names, trademarks, etc. used in this document, even when not specifically marked as such, are protected by law. PerkinElmer is a registered trademark of PerkinElmer, Inc. All other trademarks and registered trademarks not owned by PerkinElmer, Inc. or its subsidiaries that are depicted herein are the property of their respective owners. **Except as specifically set forth in its terms and conditions of sale, PerkinElmer makes no Warranty of any kind with regard to this document, including, but not limited to, the implied warranties of merchantability and fitness for a particular purpose.** PerkinElmer shall not be liable for incidental or consequential damages in connection with the furnishing or use of this document.

Component List

Component / Specific Model	Serial #	Software Version	Configuration Notes
Clarus680	680S14042502	Totalchrom6.3.2	PSS, PSS, FID,
Clarus SQ8T	648N4050804	Turbomass 6.4	
AtomX	US14113002	Tekma AtomX	

Parts Lists

Additional Tools Required for PM				
Part Number (if applicable)	Description	Quantity	Serial #	Calibration Due Date (MM/YY)
N/A				
Additional Reagents and Standards Required for PM				
Part Number (if applicable)	Description	Quantity	Batch/Lot #	Expiration Date (MM/YY)
N/A				

Procedure Checklist

Use (✓) to check off those steps in the checklist that have been completed.

1. General:

- ☒ Review the instrument performance with the customer and document any recent problems.
- ☒ Check incoming AC line voltage for proper levels and grounding.
 L-N 220 Volt
 L-G 220 Volt
 N-G 0.32 Volt

**Neutral to ground not more than 0.5 volts peak to peak*
- ☒ Inspect all gas line filters and traps; Replace if necessary with customer supplied spares.
 Carrier gas ☒ Helium ☐ Nitrogen ☐ Hydrogen
 Moisture level ☒ Good ☐ Need to replace ☐ Other _____

 Detector gas ☒ Air Zero ☒ Hydrogen ☐ Nitrogen ☐ Helium
 Moisture level ☒ Good ☐ Need to replace ☐ Other _____
- ☒ Inspect the customer log book and make any appropriate PM entries.
- ☒ Leak check all fittings from the gas source to instrument.
 Gas leakage ☒ Pass ☐ Fail Comment _____
- ☒ Perform general inspection of system for cleanliness.
- ☒ Inspect for functional and clean electronic cooling and oven vent fans
 Electronic cooling fan ☒ Yes ☐ No
 Oven cooling fan ☒ Yes ☐ No

2. Electronic :

- ☒ Check oven temperature. Calibrate if necessary.
 Oven temperature set point 150 °C ☒ Pass ☐ Fail
- ☐ Check sub-ambient option. (If installed).
 Oven temperature set point 5 °C ☐ Pass ☐ Fail
- ☒ Perform routine maintenance on detector/injector. Replace parts as necessary with customer supplied spares.

- ☒ Check flows, including split flows if applicable. Calibrate if necessary.
 Carrier flow Pass
 Split flow Pass
- ☒ Check detector gas flows and adjust if necessary.
 Detector flow Pass
- ☒ Autosampler installed ☒ Yes ☐ No
 Check autosampler sensor for wear and replace if necessary.
 Vial sensor Pass
 Door sensor Pass
 Tower sensor Pass
 Plunger sensor Pass
 Elevator sensor Pass
- ☒ Remove syringe, manually flush. Replace with customer supplied spare if necessary.
- ☒ Check firmware version. Upgrade to current levels if necessary.
 Firmware version 6.5
- ☒ Measure all accessible power supply voltages.
 5 Volt Pass
 +15 Volt Pass
 -15 Volt Pass
 24 Volt Pass
- ☒ Record all detector voltage signal.
 Detector Channel A 0.98 mV.
 Detector Channel B NA mV.

3. Diagnostics Tests:

- ☒ Run instrument diagnostics.
 BRAM Pass
 EPROM Pass
- ☒ Run Autosampler diagnostics.
 BRAM Pass
 EPROM Pass

4. Review:

- ☒ Review with the customer PM work performed.
- ☒ Review with the customer routine maintenance procedures.
- ☒ Discuss recommended customer-supplied materials to have on hand
- ☒ Attach PM sticker.
- ☒ Update Logbook.

Additional Comments

Additional Comments Regarding the PM

Review

<i>The preventive maintenance checks and if applicable performance tests for Clarus600/680 GC have been completed.</i>	
<i>This Clarus600/680 GC Pass the preventive maintenance.</i>	
Review of Preventive Maintenance:	
Authorized PerkinElmer Representative: Monchai Kitcharoenkeat <i>Monchai</i>	Date: 13-Aug-2025 (DD-MMM-YYYY)
Authorized Customer Representative: Ms.Naruecha <i>Naruecha</i>	Date: 13-Aug-2025 (DD-MMM-YYYY)

เอกสารแนบ 5-6

เอกสารสอบเทียบเครื่องมือการตรวจวัดคุณภาพอากาศในสถานประกอบการ



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจตุจักร เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chulachak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

Personal Pump Calibration Report

Calibration Method : Dry Cal Primary Flowmeter

Model : Defender 510-H

S/N : 136833

Environmental Conditions

Temperature 25 ± 3 °C
Pressure 1010 ± 15 mmbar

Personal Pump Data

Calibration Data

No.	Brand	Model	Serial No.	Date	Flow Rate (ml/min)						Value From Calibration Curve	
					Setting			Actual (Q std.)				
					1	2	3	1	2	3	y	R ²
R01	SKC	224-PCXR4	602467	02/04/2025	1,000	1,500	2,000	1,003	1,506	2,001	1.003x - 1.855	1.000
R02	SKC	224-PCXR4	626450	02/04/2025	1,000	1,500	2,000	994	1,501	2,002	1.006x - 11.866	1.000
R03	SKC	224-PCXR4	691592	01/04/2025	1,000	1,500	2,000	995	1,509	2,007	1.013x - 22.400	0.999
R04	SKC	224-PCXR4	691672	02/04/2025	1,000	1,500	2,000	996	1,502	1,996	0.999x + 0.668	1.000
R05	SKC	224-PCXR4	798470	04/04/2025	1,000	1,500	2,000	995	1,511	2,005	1.010x - 16.711	0.999
R06	SKC	224-PCXR4	798456	04/04/2025	1,000	1,500	2,000	1,002	1,499	2,003	1.004x - 5.745	1.000
R07	SKC	224-PCXR4	798480	04/04/2025	1,000	1,500	2,000	1,005	1,504	2,007	1.011x - 16.099	0.999
R08	SKC	224-PCXR4	883215	04/04/2025	1,000	1,500	2,000	1,002	1,503	2,004	1.014x - 23.623	0.999
R09	SKC	224-PCXR4	034650	02/04/2025	1,000	1,500	2,000	999	1,497	2,011	1.009x + 11.282	1.000
R10	SKC	224-PCXR4	091765	01/04/2025	1,000	1,500	2,000	1,002	1,505	2,003	1.012x - 20.705	0.999
R11	SKC	224-PCXR4	091763	02/04/2025	1,000	1,500	2,000	997	1,504	2,005	1.005x - 4.550	1.000
R12	SKC	224-PCXR4	091568	02/04/2025	1,000	1,500	2,000	998	1,513	2,004	1.015x - 25.798	0.999
R13	SKC	224-PCXR4	091638	03/04/2025	1,000	1,500	2,000	996	1,502	1,999	1.003x - 5.821	1.000
R14	SKC	224-PCXR4	091764	03/04/2025	1,000	1,500	2,000	1,002	1,503	1,997	0.997x + 5.785	1.000
R15	SKC	224-PCXR8	529437	01/04/2025	1,000	1,500	2,000	996	1,501	2,001	1.002x - 5.453	1.000
R16	SKC	224-PCXR8	529643	02/04/2025	1,000	1,500	2,000	999	1,506	1,998	0.998x + 4.829	1.000
R17	SKC	224-PCXR8	529665	02/04/2025	1,000	1,500	2,000	993	1,504	2,004	1.009x - 19.210	1.000
R18	SKC	224-PCXR8	566756	04/04/2025	1,000	1,500	2,000	1,005	1,503	2,008	1.007x - 9.639	1.000
R19	SKC	224-PCXR8	566802	04/04/2025	1,000	1,500	2,000	996	1,495	1,997	1.000x - 2.051	1.000
R20	SKC	224-PCXR8	529089	02/04/2025	1,000	1,500	2,000	999	1,498	1,999	1.004x - 12.497	1.000
R21	SKC	224-PCXR8	665728	02/04/2025	1,000	1,500	2,000	994	1,502	1,996	1.000x - 2.818	1.000
R22	SKC	224-PCXR8	707444	03/04/2025	1,000	1,500	2,000	999	1,507	2,004	1.009x - 16.603	0.999
R23	SKC	224-PCXR8	761067	03/04/2025	1,000	1,500	2,000	997	1,496	1,997	1.001x - 3.342	1.000
R24	SKC	224-PCXR8	707893	02/04/2025	1,000	1,500	2,000	1,005	1,504	2,012	1.008x - 11.430	0.999
R25	SKC	224-PCXR8	761052	01/04/2025	1,000	1,500	2,000	1,002	1,493	2,010	1.006x - 8.771	1.000
R26	SKC	224-PCXR8	707956	02/04/2025	1,000	1,500	2,000	997	1,504	1,997	1.001x - 2.663	1.000
R27	SKC	224-PCXR8	707398	02/04/2025	1,000	1,500	2,000	996	1,495	2,001	1.007x - 19.305	0.999
R28	SKC	224-PCXR8	707481	03/04/2025	1,000	1,500	2,000	1,013	1,507	2,004	0.996x + 9.887	1.000
R29	SKC	224-PCXR8	707402	04/04/2025	1,000	1,500	2,000	998	1,499	2,010	1.010x - 19.297	1.000
R30	SKC	224-PCXR8	093811	02/04/2025	1,000	1,500	2,000	1,008	1,505	2,008	1.006x - 6.261	1.000
R31	SKC	224-PCXR8	093183	02/04/2025	1,000	1,500	2,000	1,002	1,501	1,994	0.998x - 0.140	1.000
R32	SKC	224-PCXR8	671950	01/04/2025	1,000	1,500	2,000	1,001	1,498	1,997	0.997x + 3.786	1.000
R33	SKC	224-PCXR4	626254	01/04/2025	1,000	1,500	2,000	1,006	1,497	2,001	0.995x + 7.736	1.000
R34	SKC	224-PCXR4	626131	01/04/2025	1,000	1,500	2,000	994	1,506	2,006	1.009x - 17.998	1.000
R35	SKC	224-PCXR8	707460	01/04/2025	1,000	1,500	2,000	1,006	1,505	2,014	1.010x - 14.668	0.999
R36	SKC	224-PCXR0	707446	04/04/2025	1,000	1,500	2,000	998	1,500	1,995	1.000x - 2.067	1.000
R37	SKC	224-PCXR8	707432	02/04/2025	1,000	1,500	2,000	1,005	1,494	2,006	0.998x + 4.721	1.000
R38	SKC	224-PCXR8	707349	03/04/2025	1,000	1,500	2,000	996	1,511	2,007	1.012x - 19.485	0.999
R39	SKC	224-PCXR8	761095	02/04/2025	1,000	1,500	2,000	1,005	1,505	2,008	1.009x - 4.026	1.000

Calibrated by :

Adul Dangklom
(Mr. Adul Dangklom)

Approved by :

(Mr. Peera Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจตุจักร เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chulachak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

Personal Pump Calibration Report

Calibration Method : Dry Cal Primary Flowmeter

Model : Defender 510-H

S/N : 136833

Environmental Conditions

Temperature 25 ± 3 °C
Pressure 1010 ± 15 mmbar

Personal Pump Data

Calibration Data

No.	Brand	Model	Serial No.	Date	Flow Rate (ml/min)						Value From Calibration Curve	
					Setting			Actual (Q std.)			y	R ²
					1	2	3	1	2	3		
R40	SKC	224-PCXR4	612753	03/04/2025	1,000	1,500	2,000	1,013	1,505	2,008	0.996x + 6.748	0.999
R41	SKC	224-PCXR4	626140	01/04/2025	1,000	1,500	2,000	1,006	1,506	2,009	1.005x - 6.157	1.000
R42	SKC	224-PCXR4	626463	02/04/2025	1,000	1,500	2,000	1,005	1,495	2,002	0.997x + 5.089	1.000
R43	SKC	224-PCXR4	626129	04/04/2025	1,000	1,500	2,000	1,004	1,504	2,008	1.011x - 15.436	1.000
R44	SKC	224-PCXR4	602753	02/04/2025	1,000	1,500	2,000	999	1,492	2,001	1.004x - 13.988	0.999
R45	SKC	224-PCXR4	626137	03/04/2025	1,000	1,500	2,000	1,001	1,501	1,996	0.994x + 9.247	1.000

Calibrated by :

Adul Dangklom
(Mr. Adul Dangklom)

Approved by :

(Mr. Peera Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจตุจักร เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompet, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

Personal Pump Calibration Report

Calibration Method : Dry Cal Primary Flowmeter

Model : Defender 510-H

S/N : 136164

Environmental Conditions

Temperature : 25 ± 3 °C
Pressure : 1010 ± 15 mmbar

Personal Pump Data				Calibration Data									
No.	Brand	Model	Serial No.	Date	Flow Rate (ml/min)						Value From Calibration Curve		
					Setting			Actual (Q std.)					
					1	2	3	1	2	3	y		R ²
801	SKC	224-PCXR4	262101	01/07/2025	1,000	1,500	2,000	997	1,501	2,003	1.003x - 4.236	1.000	
802	SKC	224-PCXR4	626166	02/07/2025	1,000	1,500	2,000	1,005	1,506	2,007	1.001x + 1.555	1.000	
803	SKC	224-PCXR4	612968	04/07/2025	1,000	1,500	2,000	1,004	1,499	2,002	1.004x - 11.638	0.999	
804	SKC	224-PCXR4	602804	01/07/2025	1,000	1,500	2,000	999	1,502	1,998	1.002x - 3.373	1.000	
805	SKC	224-PCXR4	612693	03/07/2025	1,000	1,500	2,000	1,002	1,504	2,008	1.008x - 9.160	1.000	
806	SKC	224-PCXR4	262188	01/07/2025	1,000	1,500	2,000	1,001	1,505	2,003	1.001x - 3.965	1.000	
807	SKC	224-PCXR4	626262	02/07/2025	1,000	1,500	2,000	999	1,494	2,000	0.997x + 3.261	1.000	
808	SKC	224-PCXR4	626100	04/07/2025	1,000	1,500	2,000	1,003	1,502	2,004	1.009x - 15.922	0.999	
809	SKC	224-PCXR4	626479	01/07/2025	1,000	1,500	2,000	997	1,499	2,005	1.005x - 9.935	1.000	
810	SKC	224-PCXR4	091950	01/07/2025	1,000	1,500	2,000	995	1,507	2,001	1.008x - 15.634	1.000	
811	SKC	224-PCXR8	564515	04/07/2025	1,000	1,500	2,000	997	1,495	2,002	1.004x - 7.274	1.000	
812	SKC	224-PCXR4	034656	01/07/2025	1,000	1,500	2,000	1,001	1,507	2,005	1.007x - 13.608	0.999	
813	SKC	224-PCXR4	620273	01/07/2025	1,000	1,500	2,000	1,002	1,504	2,007	1.006x - 6.161	1.000	
814	SKC	224-PCXR4	626313	04/07/2025	1,000	1,500	2,000	999	1,503	2,004	1.001x - 3.361	1.000	
815	SKC	224-PCXR4	626474	04/07/2025	1,000	1,500	2,000	1,005	1,506	2,005	1.008x - 12.821	0.999	
816	SKC	224-PCXR4	626477	04/07/2025	1,000	1,500	2,000	997	1,509	1,995	0.999x - 0.595	1.000	
817	SKC	224-PCXR4	626860	02/07/2025	1,000	1,500	2,000	999	1,497	1,996	1.000x - 1.613	1.000	
818	SKC	224-PCXR4	691484	04/07/2025	1,000	1,500	2,000	1,003	1,499	1,995	1.003x - 9.955	0.999	
819	SKC	224-PCXR4	691599	01/07/2025	1,000	1,500	2,000	996	1,508	1,994	1.001x - 1.127	1.000	
820	SKC	224-PCXR4	691587	02/07/2025	1,000	1,500	2,000	997	1,505	1,997	1.004x - 9.596	1.000	
821	SKC	224-PCXR4	691531	03/07/2025	1,000	1,500	2,000	998	1,504	1,999	1.002x - 3.125	1.000	
822	SKC	224-PCXR4	691654	04/07/2025	1,000	1,500	2,000	1,002	1,505	1,992	1.003x - 9.240	0.999	
823	SKC	224-PCXR4	798393	01/07/2025	1,000	1,500	2,000	992	1,498	1,993	0.999x - 3.941	1.000	
824	SKC	224-PCXR4	626363	02/07/2025	1,000	1,500	2,000	1,004	1,506	1,994	1.003x - 9.084	0.999	
825	SKC	224-PCXR4	798489	03/07/2025	1,000	1,500	2,000	1,005	1,497	2,004	0.998x + 5.100	1.000	
826	SKC	224-PCXR4	798479	03/07/2025	1,000	1,500	2,000	1,004	1,504	1,998	0.997x + 5.575	1.000	
827	SKC	224-PCXR4	691673	04/07/2025	1,000	1,500	2,000	997	1,508	1,991	1.002x - 8.556	0.999	
828	SKC	224-PCXR4	691570	03/07/2025	1,000	1,500	2,000	1,005	1,504	2,001	1.000x + 2.897	1.000	
829	SKC	224-PCXR4	626472	02/07/2025	1,000	1,500	2,000	1,003	1,502	2,004	1.001x - 1.675	1.000	
830	SKC	224-PCXR4	691689	03/07/2025	1,000	1,500	2,000	1,004	1,510	2,007	1.010x - 13.764	0.999	
831	SKC	224-PCXR4	691509	02/07/2025	1,000	1,500	2,000	996	1,499	1,991	0.997x + 0.891	1.000	
832	SKC	224-PCXR4	091567	03/07/2025	1,000	1,500	2,000	998	1,497	1,996	0.996x + 3.273	1.000	
833	SKC	224-PCXR4	091756	02/07/2025	1,000	1,500	2,000	1,004	1,505	1,992	1.000x - 4.228	0.999	
834	SKC	224-PCXR4	612962	04/07/2025	1,000	1,500	2,000	1,005	1,508	2,011	1.007x - 5.447	1.000	
835	SKC	224-PCXR4	602682	02/07/2025	1,000	1,500	2,000	1,004	1,506	1,991	0.997x + 1.603	0.999	
836	SKC	224-PCXR4	626164	01/07/2025	1,000	1,500	2,000	999	1,498	2,002	1.004x - 8.113	1.000	
837	SKC	224-PCXR4	626256	02/07/2025	1,000	1,500	2,000	995	1,508	2,001	1.005x - 10.431	1.000	
838	SKC	224-PCXR4	626167	02/07/2025	1,000	1,500	2,000	1,000	1,497	1,993	0.999x - 0.639	1.000	
839	SKC	224-PCXR4	034637	04/07/2025	1,000	1,500	2,000	1,005	1,503	1,991	1.002x - 7.186	0.999	
840	SKC	224-PCXR4	798349	03/07/2025	1,000	1,500	2,000	995	1,494	1,990	1.000x - 7.405	1.000	

Calibrated by :

Adul Dangklom
(Mr. Adul Dangklom)

Approved by :

Peers Detudom
(Mr. Peers Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจตุจักร เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompet, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

Personal Pump Calibration Report

Calibration Method : Dry Cal Primary Flowmeter

Model : Defender 510-H

S/N : 136164

Environmental Conditions

Temperature : 25 ± 3 °C
Pressure : 1010 ± 15 mmbar

Personal Pump Data				Calibration Data									
No.	Brand	Model	Serial No.	Date	Flow Rate (ml/min)						Value From Calibration Curve		
					Setting			Actual (Q std.)					
					1	2	3	1	2	3	y	R ²	
841	SKC	224-PCXR4	612669	03/07/2025	1,000	1,500	2,000	999	1,498	2,001	1.001x - 3.597	1.000	
842	SKC	224-PCXR4	626041	02/07/2025	1,000	1,500	2,000	1,003	1,499	2,007	1.005x - 8.012	1.000	
843	SKC	224-PCXR4	034636	03/07/2025	1,000	1,500	2,000	1,004	1,506	1,997	0.993x + 10.787	1.000	
844	SKC	224-PCXR8	529341	02/07/2025	1,000	1,500	2,000	1,002	1,502	2,009	1.010x - 14.387	1.000	
845	SKC	224-PCXR8	529594	03/07/2025	1,000	1,500	2,000	999	1,509	1,991	0.992x + 12.045	1.000	
846	SKC	224-PCXR8	566743	03/07/2025	1,000	1,500	2,000	998	1,505	2,000	1.006x - 13.608	0.999	
847	SKC	224-PCXR8	566747	03/07/2025	1,000	1,500	2,000	1,002	1,504	1,998	1.004x - 7.545	1.000	
848	SKC	224-PCXR8	566753	02/07/2025	1,000	1,500	2,000	998	1,494	1,996	0.998x - 0.387	1.000	
849	SKC	224-PCXR8	566780	04/07/2025	1,000	1,500	2,000	1,002	1,499	1,995	1.005x - 13.932	0.999	
850	SKC	224-PCXR8	500400	03/07/2025	1,000	1,500	2,000	1,006	1,498	2,008	1.002x - 1.667	1.000	
851	SKC	224-PCXR8	590363	04/07/2025	1,000	1,500	2,000	999	1,505	2,002	1.008x - 17.209	0.999	
852	SKC	224-PCXR8	093186	02/07/2025	1,000	1,500	2,000	994	1,496	1,998	1.003x - 7.976	1.000	
853	SKC	224-PCXR8	707670	02/07/2025	1,000	1,500	2,000	997	1,512	2,002	1.004x - 6.981	1.000	
854	SKC	224-PCXR3	509821	02/07/2025	1,000	1,500	2,000	1,002	1,503	2,006	1.009x - 17.041	0.999	
855	SKC	224-PCXR3	510710	04/07/2025	1,000	1,500	2,000	1,000	1,501	1,993	0.996x + 2.606	1.000	
856	SKC	224-PCXR3	511450	02/07/2025	1,000	1,500	2,000	1,012	1,502	2,008	0.997x + 9.801	1.000	
857	SKC	224-PCXR3	510798	01/07/2025	1,000	1,500	2,000	1,001	1,493	2,004	1.003x - 2.925	1.000	
858	SKC	224-PCXR3	509852	04/07/2025	1,000	1,500	2,000	1,004	1,499	1,997	1.001x - 8.640	0.999	
859	SKC	224-PCXR3	509862	04/07/2025	1,000	1,500	2,000	1,000	1,504	2,001	0.999x + 4.160	1.000	
860	SKC	224-PCXR3	512655	01/07/2025	1,000	1,500	2,000	1,005	1,502	2,008	1.007x - 9.991	1.000	
861	SKC	224-PCXR3	503915	03/07/2025	1,000	1,500	2,000	995	1,491	1,995	1.003x - 8.373	1.000	
862	SKC	224-PCXR3	505975	03/07/2025	1,000	1,500	2,000	1,003	1,498	2,001	1.002x - 4.813	1.000	
863	SKC	224-PCXR3	511432	01/07/2025	1,000	1,500	2,000	995	1,503	1,996	1.008x - 19.707	0.999	
864	SKC	224-PCXR3	509302	01/07/2025	1,000	1,500	2,000	999	1,494	1,992	0.993x + 6.854	1.000	
865	SKC	224-PCXR3	508310	01/07/2025	1,000	1,500	2,000	1,000	1,505	2,001	1.003x - 8.089	0.999	
866	SKC	224-PCXR3	509861	02/07/2025	1,000	1,500	2,000	1,002	1,495	1,996	0.992x - 10.934	1.000	
867	SKC	224-PCXR3	506295	03/07/2025	1,000	1,500	2,000	995	1,509	1,997	1.001x - 4.236	1.000	
868	SKC	224-PCXR3	505872	03/07/2025	1,000	1,500	2,000	1,001	1,491	2,001	1.000x - 1.187	1.000	
869	SKC	224-PCXR3	508375	04/07/2025	1,000	1,500	2,000	1,006	1,505	1,998	1.005x - 11.342	0.999	
870	SKC	224-PCXR3	510623	03/07/2025	1,000	1,500	2,000	997	1,508	1,997	1.001x - 1.890	1.000	
871	SKC	224-PCXR3	508367	02/07/2025	1,000	1,500	2,000	1,001	1,506	2,004	1.006x - 12.521	0.999	
872	SKC	224-PCXR3	505977	01/07/2025	1,000	1,500	2,000	1,007	1,496	1,998	0.991x + 11.538	1.000	
873	SKC	224-PCXR3	512606	01/07/2025	1,000	1,500	2,000	1,002	1,498	1,995	0.996x + 0.711	1.000	
874	SKC	224-PCXR3	505993	01/07/2025	1,000	1,500	2,000	999	1,497	1,998	1.002x - 6.570	1.000	
875	SKC	224-PCXR3	509820	02/07/2025	1,000	1,500	2,000	998	1,499	1,996	0.999x - 0.923	1.000	
876	SKC	224-PCXR3	509811	02/07/2025	1,000	1,500	2,000	997	1,502	2,003	1.007x - 11.834	1.000	
877	SKC	224-PCXR3	508301	04/07/2025	1,000	1,500	2,000	1,005	1,505	1,993	1.000x - 3.349	0.999	
878	SKC	224-PCXR3	510677	04/07/2025	1,000	1,500	2,000	999	1,509	1,998	1.004x - 9.791	0.999	
879	SKC	224-PCXR3	510920	02/07/2025	1,000	1,500	2,000	998	1,498	1,994	0.997x + 2.162	1.000	



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจตุจักร เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

Personal Pump Calibration Report

Calibration Method : Dry Cal Primary Flowmeter

Model : Defender 510-H

S/N : 136164

Environmental Conditions

Temperature : 25 ± 3 °C
Pressure : 1010 ± 15 mmbar

Personal Pump Data

Calibration Data

Personal Pump Data				Calibration Data								
No.	Brand	Model	Serial No.	Date	Flow Rate (ml/min)						Value From Calibration Curve	
					Setting			Actual (Q std.)				
					1	2	3	1	2	3	y	R ²
B80	SKC	224-PCXR3	504569	01/07/2025	1,000	1,500	2,000	1,005	1,501	2,007	1.014x - 22.484	0.999
B81	SKC	224-PCXR3	503480	02/07/2025	1,000	1,500	2,000	997	1,494	1,995	1.005x - 14.583	1.000
B82	SKC	224-PCXR3	505673	04/07/2025	1,000	1,500	2,000	998	1,497	2,001	1.004 - 6.075	1.000
B83	SKC	224-PCXR3	510785	04/07/2025	1,000	1,500	2,000	1,009	1,501	1,998	1.003x - 7.370	0.999
B84	SKC	224-PCXR3	508333	02/07/2025	1,000	1,500	2,000	997	1,502	1,997	1.000x - 1.894	1.000
B85	SKC	224-PCXR3	505757	02/07/2025	1,000	1,500	2,000	1,002	1,503	2,004	1.004x + 7.222	1.000
B86	SKC	224-PCXR3	512625	01/07/2025	1,000	1,500	2,000	999	1,493	1,997	0.996x + 1.139	1.000
B87	SKC	224-PCXR3	504324	01/07/2025	1,000	1,500	2,000	1,001	1,498	2,002	1.001x + 0.607	1.000
B88	SKC	224-PCXR3	508307	02/07/2025	1,000	1,500	2,000	999	1,497	1,995	0.995x + 5.331	1.000
B89	SKC	224-PCXR3	509860	02/07/2025	1,000	1,500	2,000	1,003	1,494	1,998	1.007x - 15.027	0.999
B90	SKC	224-PCXR3	508366	04/07/2025	1,000	1,500	2,000	997	1,510	1,992	0.998x + 0.332	1.000
B91	SKC	224-PCXR3	510919	03/07/2025	1,000	1,500	2,000	1,005	1,503	1,999	0.990x + 13.532	1.000
B92	SKC	224-PCXR3	510987	03/07/2025	1,000	1,500	2,000	1,004	1,506	2,002	0.999x + 3.737	1.000
B93	SKC	224-PCXR3	509845	03/07/2025	1,000	1,500	2,000	997	1,501	2,004	1.008x - 12.857	1.000

Calibrated by :

Adul Dengklom
(Mr. Adul Dengklom)

Approved by :

Peera Detudom
(Mr. Peera Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chulachak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4321, E-mail : sale@spacon.com, www.spacon.com

Rotameter Calibration Report (For Personal Pump High Flow Adjust)

Calibration Method : Dry Cal Primary Flowmeter

Model : Defender 510-H

S/N : 136164

Calibration Data

Rotameter Data			Calibration Data								
No.	Brand	Model	Date	Flow Rate (mL/min)						Value From Calibration Curve	
				Flow Rate (Reading)			Actual (Q std.)			y	R ²
				1	2	3	1	2	3		
H-R01	Dwyer	VFB-65	02/04/2025	500	1,000	2,000	499.6	998.8	2004.8	1.001x - 3.678	1.000
H-R02	Dwyer	VFB-65	02/04/2025	500	1,000	2,000	501.7	997.1	1991.5	0.998x + 0.386	0.999
H-R03	Dwyer	VFB-65	01/04/2025	500	1,000	2,000	499.8	999.7	1992.8	1.000x + 1.316	1.000
H-R04	Dwyer	VFB-65	04/04/2025	500	1,000	2,000	500.2	999.4	1989.2	0.999x + 1.870	0.999
H-R05	Dwyer	VFB-65	04/04/2025	500	1,000	2,000	499.9	1000.8	1994.5	1.000x + 0.815	1.000
H-R06	Dwyer	VFB-65	03/04/2025	500	1,000	2,000	500.5	1001.3	1990.7	0.997x + 4.894	0.999

Calibrated by :

Adul Dangklom
(Mr Adul Dangklom)

Approved by :

Mr. Peera Detudom
(Mr. Peera Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chulachak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4321, E-mail : sale@spacon.com, www.spacon.com

Rotameter Calibration Report (For Personal Pump Low Flow Adjust)

Calibration Method : Dry Cal Primary Flowmeter

Model : Defender 510-H

S/N : 136164

Calibration Data

Rotameter Data			Calibration Data								
No.	Brand	Model	Date	Flow Rate (mL/min)						Value From Calibration Curve	
				Flow Rate (Reading)			Actual (Q std.)			y	R ²
				1	2	3	1	2	3		
L-R01	Dwyer	VFA-21	02/04/2025	50	100	200	50.7	101.0	199.3	0.995x + 1.197	1.000
L-R02	Dwyer	VFA-21	02/04/2025	50	100	200	49.8	100.7	199.1	1.001x - 0.303	1.000
L-R03	Dwyer	VFA-21	01/04/2025	50	100	200	50.1	101.2	200.9	1.005x - 0.447	0.999
L-R04	Dwyer	VFA-21	04/04/2025	50	100	200	50.2	100.9	201.5	0.994x + 1.311	1.000
L-R05	Dwyer	VFA-21	04/04/2025	50	100	200	50.4	100.7	201.6	0.999x + 0.781	1.000
L-R06	Dwyer	VFA-21	03/04/2025	50	100	200	49.8	101.2	201.8	1.003x - 0.149	0.999

Calibrated by :

Adul Dangklom
(Mr Adul Dangklom)

Approved by :

Mr. Peera Detudom
(Mr. Peera Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72 Fax : (662) 513-4221 E-mail : sale@spscon.com, www.spscon.com

Rotameter Calibration Report (For Personal Pump High Flow Adjust)

Calibration Method : Dry Cal Primary Flowmeter

Model : Defender 510-H

S/N : 136164

Calibration Data

Rotameter Data			Calibration Data								
No.	Brand	Model	Date	Flow Rate (mL/min)						Value From Calibration Curve	
				Flow Rate (Reading)			Actual (Q std.)				
				1	2	3	1	2	3	y	R ²
H-R01	Dwyer	VFB-65	04/01/2025	500	1,000	2,000	500.4	999.6	2002.7	0.999x + 1.975	1.000
H-R02	Dwyer	VFB-65	04/01/2025	500	1,000	2,000	499.3	998.9	1998.1	1.000x - 0.723	1.000
H-R03	Dwyer	VFB-65	03/01/2025	500	1,000	2,000	500.5	998.7	1996.7	0.998x + 2.184	0.999
H-R04	Dwyer	VFB-65	02/01/2025	500	1,000	2,000	501.7	998.1	1993.3	1.000x - 2.212	0.999
H-R05	Dwyer	VFB-65	02/01/2025	500	1,000	2,000	499.2	997.5	1997.1	1.002x - 3.115	1.000
H-R06	Dwyer	VFB-65	02/01/2025	500	1,000	2,000	499.8	997.4	1993.2	1.001x - 4.372	0.999

Calibrated by :

Adul Dangklom

(Mr. Adul Dangklom)

Approved by :

Mr. Peera Detudom

(Mr. Peera Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72 Fax : (662) 513-4221 E-mail : sale@spscon.com, www.spscon.com

Rotameter Calibration Report (For Personal Pump Low Flow Adjust)

Calibration Method : Dry Cal Primary Flowmeter

Model : Defender 510-H

S/N : 136164

Calibration Data

Rotameter Data				Calibration Data							
No.	Brand	Model	Date	Flow Rate (mL/min)						Value From Calibration Curve	
				Flow Rate (Reading)			Actual (Q std.)				
				1	2	3	1	2	3	y	R ²
L-R01	Dwyer	VFA-21	04/01/2025	50	100	200	50.9	100.4	201.3	1.001x + 0.676	1.000
L-R02	Dwyer	VFA-21	04/01/2025	50	100	200	50.3	101.8	201.0	1.003x + 0.005	0.999
L-R03	Dwyer	VFA-21	03/07/2025	50	100	200	50.6	100.9	201.1	0.999x + 0.565	1.000
L-R04	Dwyer	VFA-21	02/07/2025	50	100	200	50.5	100.4	200.8	0.997x + 0.797	1.000
L-R05	Dwyer	VFA-21	02/07/2025	50	100	200	50.1	101.7	200.9	1.002x - 0.024	0.999
L-R06	Dwyer	VFA-21	02/07/2025	50	100	200	50.3	101.5	200.8	1.000x + 0.647	1.000

Calibrated by :

Adul Dangklom

(Mr. Adul Dangklom)

Approved by :

Mr. Peera Detudom

(Mr. Peera Detudom)



บริษัท ไทยยูนิค จำกัด

THAI UNIQUE CO., LTD.

80-82 ถนนประชาธิปไตย แขวงบางขุนพรหม เขตพระนคร กรุงเทพฯ 10200

80-82 Prachathipatai Rd., Bangkhunphrom, Pranakorn, Bangkok 10200

Tel. 0-2629-0191-6, 0-2280-1787, Fax. 0-2280-1788, E-mail : thawatt@thaiunique.com, Website : www.thaiunique.com

GAS CHROMATOGRAPH TEST CERTIFICATION

Certificate No. : SV0825/23032

Instrument Type : Gas Chromatography

Model : 3800

Serial Number : 00734

Organization : S.P.S. Consulting Service Co., Ltd.

Address : 7 Phahonyothin Soi 24 Phahonyothin Rd. Ladyao Chatuchak Bangkok 10900

Date : 02/08/2025

ELECTRONIC TEST

CPU	<input checked="" type="checkbox"/> PASS	<input type="checkbox"/> FAIL
DISPLAY & LED TEST	<input checked="" type="checkbox"/> PASS	<input type="checkbox"/> FAIL
VENT TEST	<input checked="" type="checkbox"/> PASS	<input type="checkbox"/> FAIL
KEY ECHO TEST	<input checked="" type="checkbox"/> PASS	<input type="checkbox"/> FAIL
DESTRUCTION RAM TEST	<input checked="" type="checkbox"/> PASS	<input type="checkbox"/> FAIL

RUN CHROMATOGRAM TEST

DETECTOR : Flame Ionization Detectors (FID Channel-Front)

INJECTOR : 1079 Injector

GC CONDITION:

Column	80 °C hold 1 min., rate 20 °C/min. to 200 °C hold 1min.
Injector	220 °C
Detector	300 °C
Column flow	5 mL/min
Makeup flow	25 mL/min
Air flow	300 mL/min
Hydrogen flow	30 mL/min

Column:Capillary Column CP sil 5 CB 0.25 ID x 15 M

Sample: 1 µL Injection FID Test Sample 0.218g/L C14,C15,C16 in hexane (diluted to 30ppm)

SENSITIVITY TEST: C15. (Area count) = 515,940 Counts.



บริษัท ไทยยูนิค จำกัด

THAI UNIQUE CO., LTD.

80-82 ถนนประชาธิปไตย แขวงบางขุนพรหม เขตพระนคร กรุงเทพฯ 10200

80-82 Prachathipatai Rd., Bangkhunphrom, Pranakorn, Bangkok 10200

Tel. 0-2629-0191-6, 0-2280-1787, Fax. 0-2280-1788, E-mail : thawatt@thaiunique.com, Website : www.thaiunique.com

Detector Sensitivity (FID)

Detector Response	Result	Specification
Baseline Noise (µV)	2.40	≤ 50
Baseline Drift (%)	0.18	≤ 1
Sensitivity (S/N for C15)	19,716	≥ 1,024


Temperature Specification

Temperature	Set	Result	Specification
Column Oven (°C)	80	79	± 5
Injector (°C)	220	218	± 5
Detector (°C)	300	298	± 5
Incubator (°C)	60	N/A	± 5

Relative Standard Deviation % (%RSD)

Checkout Procedure	Result	Specification
Area C15 (%)	1.48	≤ 5
Retention Time C15 (%)	0.08	≤ 0.5

APPROVAL:

Signature: 

Engineer : Somchai Pohtongkam

Date : 02/08/2025



VARIAN

1/2

SERVICE DEPARTMENT

FR-SV-029 Rev. 04



VARIAN

2/2

SERVICE DEPARTMENT

FR-SV-029 Rev. 04



บริษัท ไทยยูนิค จำกัด THAI UNIQUE CO., LTD.

80-82 ถนนประชาธิปไตย แขวงบางขุนพรหม เขตพระนคร กรุงเทพฯ 10200
80-82 Prachathipatai Rd., Bangkhunphrom, Pranakorn, Bangkok 10200

Tel. 0-2629-0191-6, 0-2280-1787, Fax. 0-2280-1788, E-mail : thawatt@thaiunique.com, Website : www.thaiunique.com

Results Integrated System Testing

Checkout Procedure	FID
Detector Position	Front
Inlet Type	1079 Injector
C15 Area 1	506,043
C15 Area 2	520,497
C15 Area 3	522,154
C15 Area 4	521,664
C15 Area 5	509,340
C15 Area Average	515,940
* % RSD (< 5 %)	1.48

* The precision specification should be less than 2.0 % RSD ** (Relative Standard Deviation) for an Auto sampler injection and less than 5 % for Manual injections. To calculate the %RSD, select the C15 peak area for each of the five (5) samples.

** (Relative Standard Deviation is determined by dividing the standard deviation by the average and multiplying by 100.)

$$\% \text{ RSD} = (\text{std.dev} / \text{avg}) * 100$$

Compliance	<input checked="" type="checkbox"/> Pass	<input type="checkbox"/> Fail
Performance by	Sankul P.	
Date	02/08/2025	



Comments			
Reviewed by	Wattana	Date	02/08/2025



บริษัท ไทยยูนิค จำกัด THAI UNIQUE CO., LTD.

80-82 ถนนประชาธิปไตย แขวงบางขุนพรหม เขตพระนคร กรุงเทพฯ 10200
80-82 Prachathipatai Rd., Bangkhunphrom, Pranakorn, Bangkok 10200

Tel. 0-2629-0191-6, 0-2280-1787, Fax. 0-2280-1788, E-mail : thawatt@thaiunique.com, Website : www.thaiunique.com

Results Integrated System Testing

Checkout Procedure	FID
Detector Position	Front
Inlet Type	1079 Injector
C15 RT 1	3.874
C15 RT 2	3.880
C15 RT 3	3.875
C15 RT 4	3.872
C15 RT 5	3.878
C15 RT Average	3.876
* % RSD (< 0.5 %)	0.08

* The precision specification should be less than 0.5 % RSD ** (Relative Standard Deviation) for an Auto sampler injection and less than 0.5 % for Manual injections. To calculate the %RSD, select the RT C15 peak for each of the five (5) samples.

** (Relative Standard Deviation is determined by dividing the standard deviation by the average and multiplying by 100.)

$$\% \text{ RSD} = (\text{std.dev} / \text{avg}) * 100$$

Compliance	<input checked="" type="checkbox"/> Pass	<input type="checkbox"/> Fail
Performance by	Sankul P.	
Date	02/08/2025	



Comments			
Reviewed by	Wattana	Date	02/08/2025



VARIAN

1/1

SERVICE DEPARTMENT



VARIAN

1/1

SERVICE DEPARTMENT


Title :
Run File : e:\sps2025\blk001.run
Method File : c:\star\data\tu\2025\cal fid.mth
Sample ID : blk

Injection Date: 2/8/2568 12:01 Calculation Date: 2/8/2568 12:33

Operator : watsamon Detector Type: 3800 (10 Volts)
Workstation: GC-LAB Bus Address : 44
Instrument : Sample Rate : 10.00 Hz
Channel : Front = FID Run Time : 20.005 min

** LC Workstation Version 6.20 ** 02511-7390-ae7-0265 **

Chart Speed = 1.13 cm/min Attenuation = 1 Zero Offset = 50%
Start Time = 0.000 min End Time = 20.005 min Min / Tick = 1.00

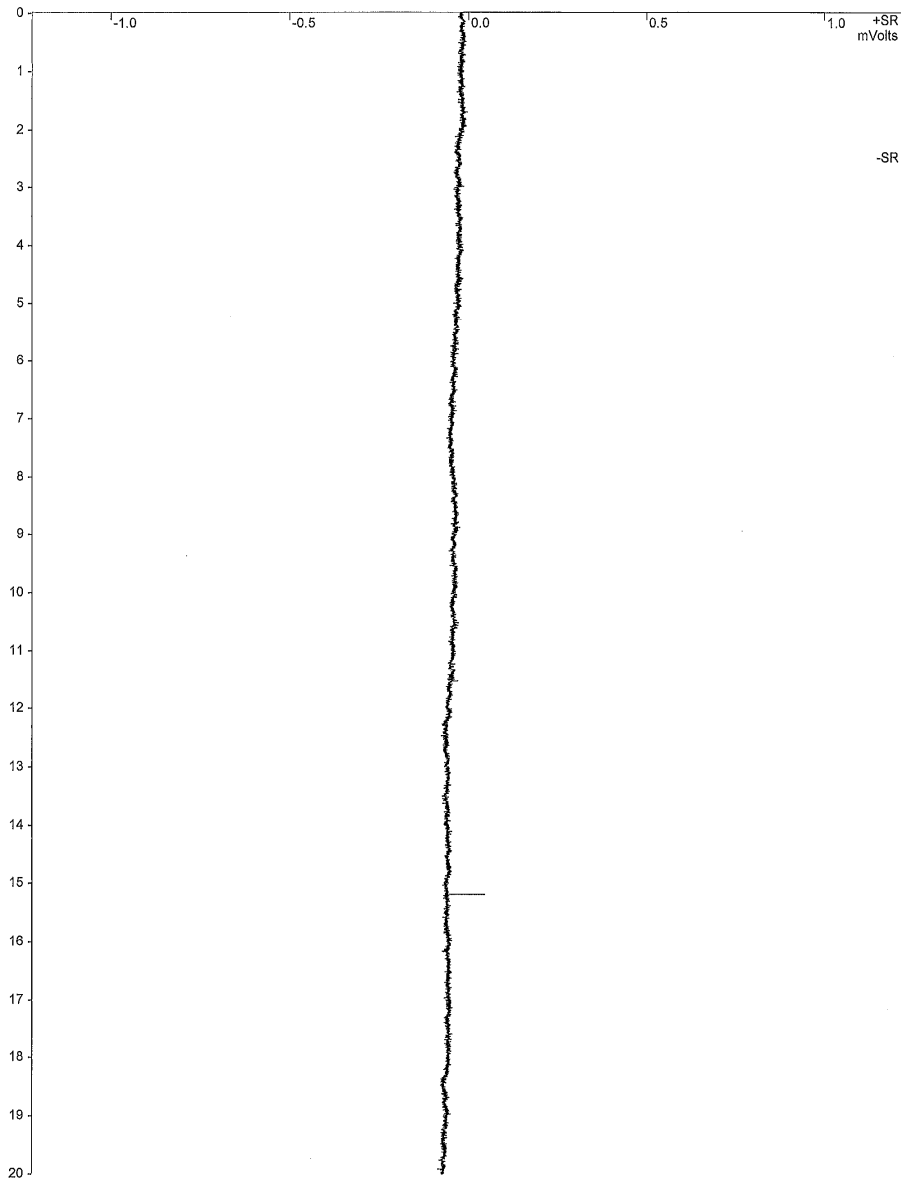

Title :
Run File : e:\sps2025\blk001.run
Method File : c:\star\data\tu\2025\cal fid.mth
Sample ID : blk

Injection Date: 2/8/2568 12:01 Calculation Date: 2/8/2568 12:33

Operator : watsamon Detector Type: 3800 (10 Volts)
Workstation: GC-LAB Bus Address : 44
Instrument : Sample Rate : 10.00 Hz
Channel : Front = FID Run Time : 20.005 min

** LC Workstation Version 6.20 ** 02511-7390-ae7-0265 **

Run Mode : Analysis
Peak Measurement: Peak Area
Calculation Type: External Standard

Peak No.	Peak Name	Result ()	Ret. Time (min)	Time Offset (min)	Area (counts)	Sep. Code	Width 1/2 (sec)	Status Codes
Totals:		0.0000		0.000	0			

Total Unidentified Counts : 0 counts

Detected Peaks: 0 Rejected Peaks: 0 Identified Peaks: 0

Multiplier: 1 Divisor: 1 Unidentified Peak Factor: 0

Baseline Offset: -14 microVolts LSB: 1 microVolts

Noise (used): 24 microVolts - monitored before this run

Manual injection

Data Handling: No peaks


Title :
Run File : e:\sps2025\fidstd001.run
Method File : c:\star\data\tu\2025\cal fid.mth
Sample ID : fidstd

Injection Date: 2/8/2568 12:34 Calculation Date: 2/8/2568 13:26

Operator : watsamon Detector Type: 3800 (10 Volts)
Workstation: GC-LAB Bus Address : 44
Instrument : Sample Rate : 10.00 Hz
Channel : Front = FID Run Time : 7.993 min

** LC Workstation Version 6.20 ** 02511-7390-ae7-0265 **

Chart Speed = 2.83 cm/min Attenuation = 79 Zero Offset = 2%
Start Time = 0.000 min End Time = 7.993 min Min / Tick = 1.00

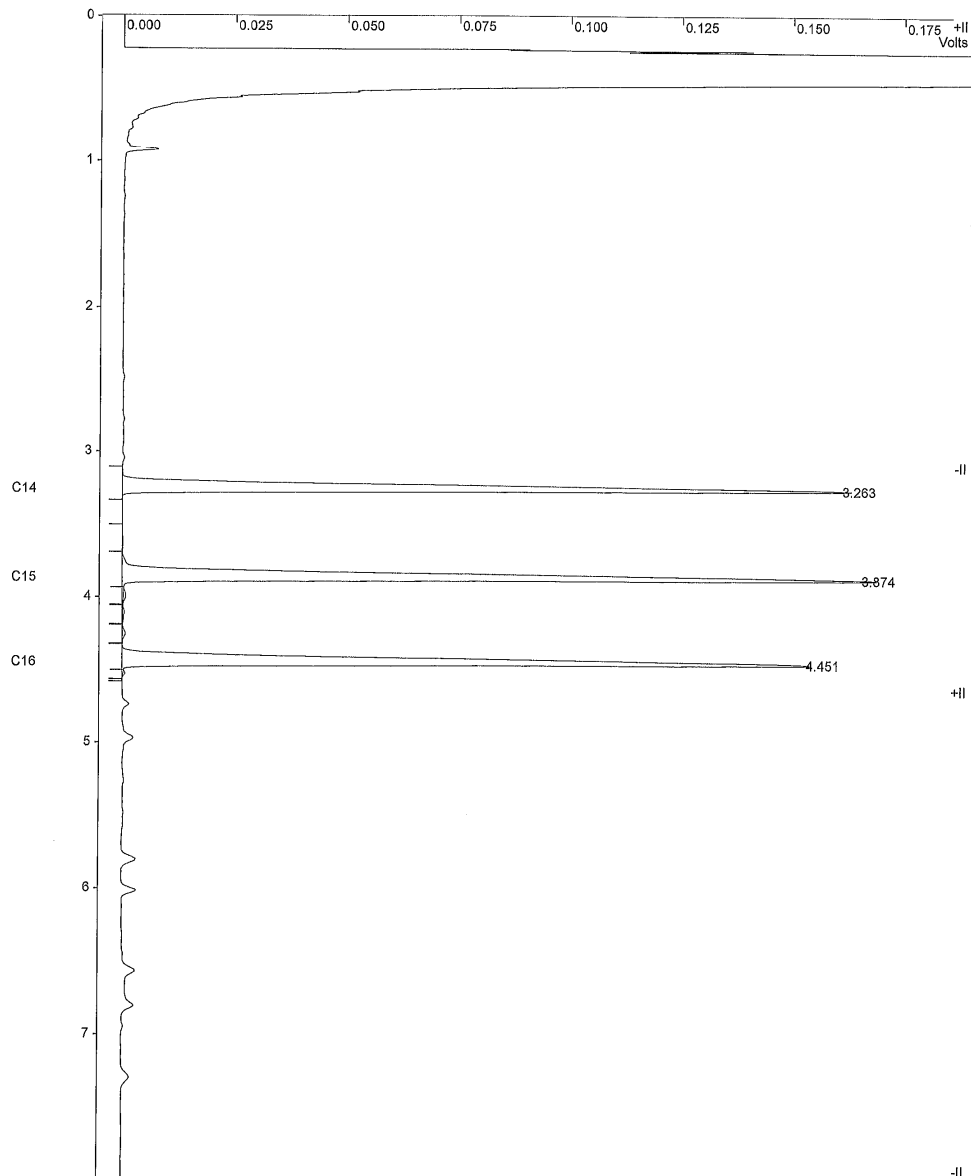

Print Date: Sat Aug 02 15:10:09 2025

Page 1 of 1

Title :
Run File : e:\sps2025\fidstd001.run
Method File : c:\star\data\tu\2025\cal fid.mth
Sample ID : fidstd

Injection Date: 2/8/2568 12:34 Calculation Date: 2/8/2568 13:26

Operator : watsamon Detector Type: 3800 (10 Volts)
Workstation: GC-LAB Bus Address : 44
Instrument : Sample Rate : 10.00 Hz
Channel : Front = FID Run Time : 7.993 min

** LC Workstation Version 6.20 ** 02511-7390-ae7-0265 **

Run Mode : Calibration
Peak Measurement: Peak Area
Calculation Type: External Standard
Level : 1

Peak No.	Peak Name	Ret. Time (min)	Time Offset (min)	Area (counts)	Sep. Code	Width 1/2 (sec)	Status Codes
1	C14	3.263	0.002	458627	BB	2.7	
2	C15	3.874	0.002	506043	VV	2.8	
3	C16	4.451	0.001	460610	VB	2.8	
Totals:			0.005	1425280			

Total Unidentified Counts : 0 counts

Detected Peaks: 8 Rejected Peaks: 5 Identified Peaks: 3

Multiplier: N/A Divisor: N/A Unidentified Peak Factor: 0


Baseline Offset: 6 microVolts LSB: 1 microVolts

Noise (used): 2 microVolts - monitored before this run

Manual injection


Sample ID: fid std

Operator (Inj): watsamon
Injection Date: 02/08/2025
Calc Date: 02/08/2025
Run Time (min): 7.993
Workstation: GC-LAB
Instrument (Inj):


VARIAN
Run Mode: Calibration
Peak Measurement: Peak Area
Calculation Type: External Std.

e:\sps2025\fidstd001.run


A = FID 10 V RESULTS

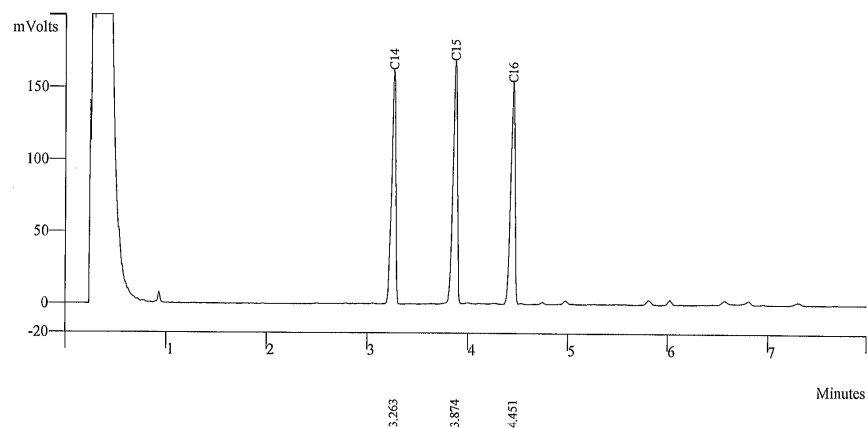

Peak No	Peak Name	Result ()	Ret Time (min)	Peak Area (counts)	Sep. Code	Width 1/2 (sec)
1	C14	0.0000	3.263	458627	BB	2.7
2	C15	0.0000	3.874	506043	VV	2.8
3	C16	0.0000	4.451	460610	VB	2.8
Totals		0.0000		1425280		


Sample ID: fid std

Operator (Inj): watsamon
Injection Date: 02/08/2025
Calc Date: 02/08/2025
Run Time (min): 7.993
Workstation: GC-LAB
Instrument (Inj):


VARIAN
Run Mode: Calibration
Peak Measurement: Peak Area
Calculation Type: External Std.

e:\sps2025\fidstd002.run

A = FID 10 V RESULTS

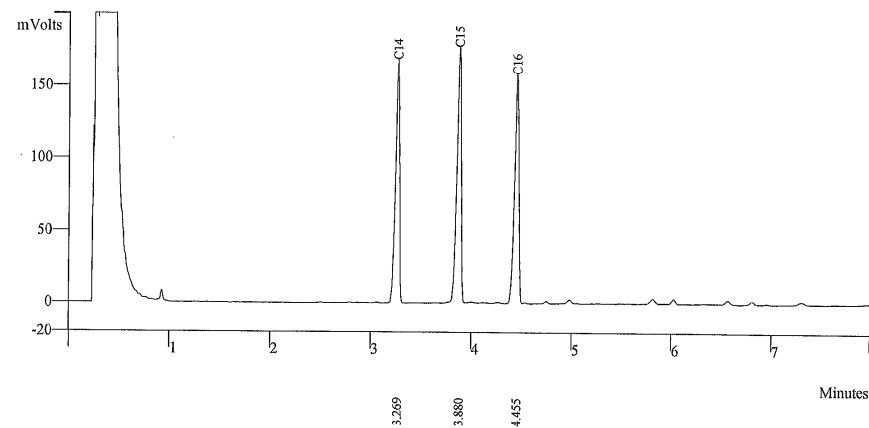

Peak No	Peak Name	Result ()	Ret Time (min)	Peak Area (counts)	Sep. Code	Width 1/2 (sec)
1	C14	0.0000	3.269	472338	BB	2.6
2	C15	0.0000	3.880	520497	VV	2.7
3	C16	0.0000	4.455	471916	VB	2.8
Totals		0.0000		1464751		

Sample ID: fid std


Operator (Inj): watsamon
Injection Date: 02/08/2025
Calc Date: 02/08/2025
Run Time (min): 7.993
Workstation: GC-LAB
Instrument (Inj):

**VARIAN**

Run Mode: Calibration
Peak Measurement: Peak Area
Calculation Type: External Std.

e:\sps2025\fidstd003.run

A = FID 10 V RESULTS

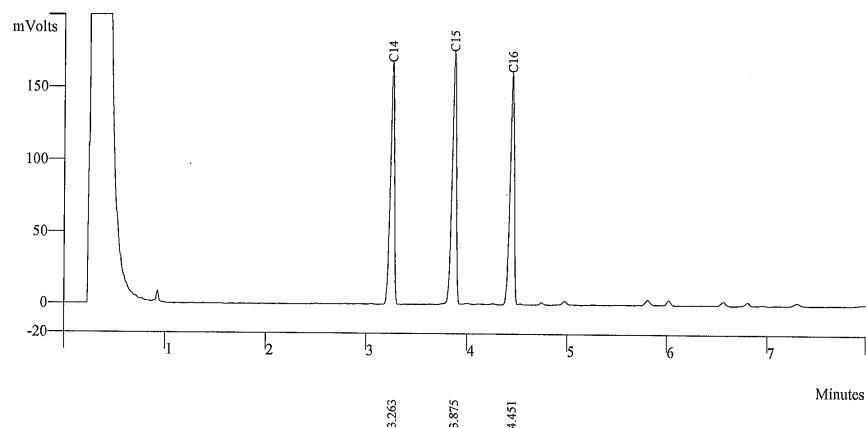

Peak No	Peak Name	Result ()	Ret Time (min)	Peak Area (counts)	Sep. Code	Width 1/2 (sec)
1	C14	0.0000	3.263	469265	BB	2.6
2	C15	0.0000	3.875	522154	VV	2.8
3	C16	0.0000	4.451	478526	VB	2.8
Totals		0.0000		1469945		



Sample ID: fid std


Operator (Inj): watsamon
Injection Date: 02/08/2025
Calc Date: 02/08/2025
Run Time (min): 7.993
Workstation: GC-LAB
Instrument (Inj):

**VARIAN**

Run Mode: Calibration
Peak Measurement: Peak Area
Calculation Type: External Std.

e:\sps2025\fidstd004.run

A = FID 10 V RESULTS

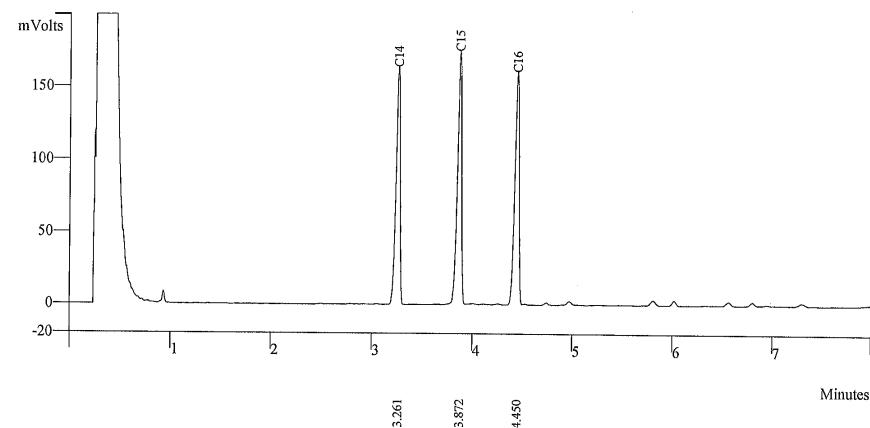

Peak No	Peak Name	Result ()	Ret Time (min)	Peak Area (counts)	Sep. Code	Width 1/2 (sec)
1	C14	0.0000	3.261	468907	BB	2.7
2	C15	0.0000	3.872	521664	VV	2.8
3	C16	0.0000	4.450	478772	VB	2.8
Totals		0.0000		1469343		



Sample ID: **fid std**


Operator (Inj): watsamon
Injection Date: 02/08/2025
Calc Date: 02/08/2025
Run Time (min): 7.993
Workstation: GC-LAB
Instrument (Inj):



Run Mode: Calibration
Peak Measurement: Peak Area
Calculation Type: External Std.

e:\sps2025\fidstd005.run

A = FID 10 V RESULTS

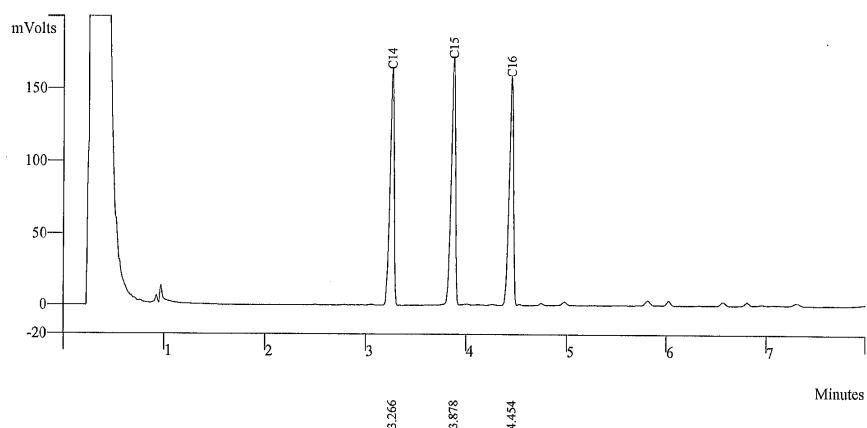

Peak No	Peak Name	Result ()	Ret Time (min)	Peak Area (counts)	Sep. Code	Width 1/2 (sec)
1	C14	0.0000	3.266	459351	BB	2.6
2	C15	0.0000	3.878	509340	VV	2.8
3	C16	0.0000	4.454	468353	VB	2.8
Totals		0.0000		1437044		




Print Date: 02 Aug 2025 15:12:58
Calibration Curves Report
File: e:\sps2025\cal fid.mth
Detector: 3800 GC, Address: 44, Channel ID: Front

C14

External Standard Analysis
Curve Type: Linear
Origin: Force
 $y = +1.552325e+004x$


Resp. Fact. RSD: 1.347%
Coeff. Det.(r²): 0.999130

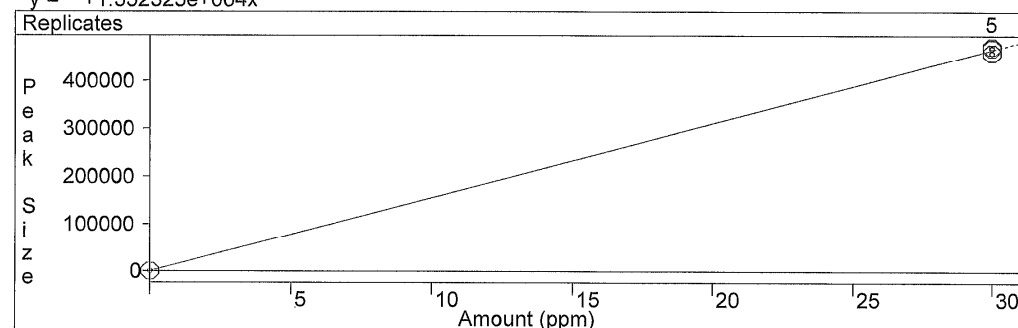

C15

External Standard Analysis
Curve Type: Linear
Origin: Force
 $y = +1.719798e+004x$


Resp. Fact. RSD: 1.481%
Coeff. Det.(r²): 0.998948

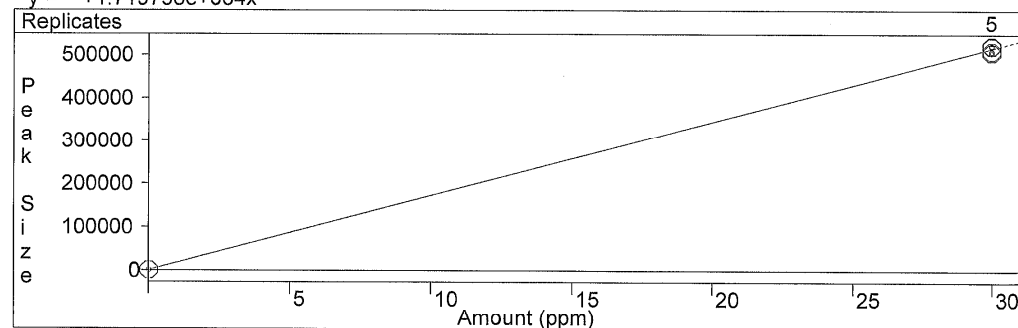

C16

External Standard Analysis
Curve Type: Linear
Origin: Force
 $y = +1.572118e+004x$

Resp. Fact. RSD: 1.611%
Coeff. Det.(r²): 0.998756

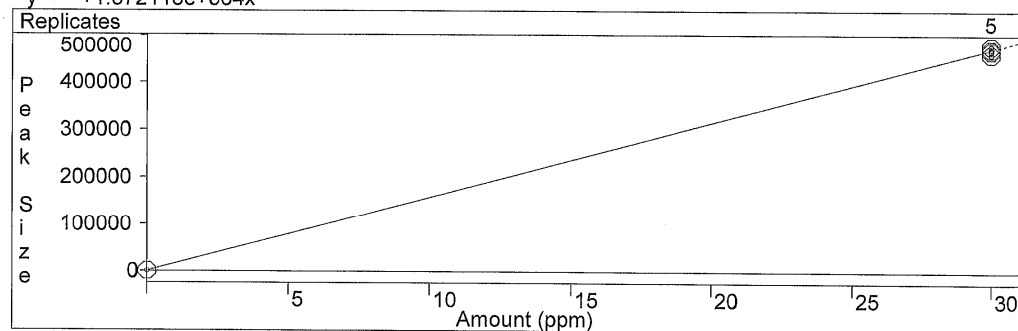

CERTIFICATE

This is to certify, that

Somchai Pohthongkham


has participated the course

Basic GC and Sampler training

Date: **24 – 27 May 2004**

Location: **Middelburg**

Instructor: **W.J. Buys**

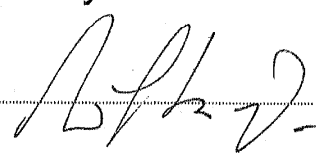Signature instructor: 



Varian Analytical Instruments
Varian Chrompack International BV
Herculesweg 8
P.O. Box 8033
4330 EA Middelburg
The Netherlands
Tel.: +31 118 671000
Fax: +31 118 633118
www.varianinc.com



WK Electric Co., Ltd.

68/242 Moo 5, Sawalpracharaj Rd., Tumbol Ladsawai, Amphur Lamlukka, Pathumthani 12150
Tel. +66 2993 4773, +66 2153 7132-3 Fax. +66 2994 5509 E-mail : wk.calibrations@gmail.com www.wk-etc.com



Certificate of Calibration

Certificate No.: WK2412-053-1

Page 1 of 2

Customer : THAI UNIQUE CO., LTD.
80-82 Prachathipatai Rd., Bangkhunphrom,
Pranakorn, Bangkok 10200

Instrument : AMD Flow Meter
Manufacturer : Agilent Technologies
Model : G6691A
Serial No. : MY16470347
Identity No. : SV-DF-001
Range : 0 ml/min to 750 ml/min
Resolution : See to Data
Calibration Method : CP-WK-M10

Ambient Temperature : (23 ± 2) °C
Humidity : (50 ± 15) %RH
Received Date : 4-Dec-24
Calibrated Date : 11-Dec-24
Issued Date : 13-Dec-24
Calibrated Location : In Lab

Reference standard instruments :

Instrument	Serial No.	Certificate No.	Due Date	Traceability to
Flow Calibrator	140215-134	L202304114-001	18-Apr-25	MIT
Primary Flow Calibrator	1107-S	WK2405-049-5	22-May-25	WK Electric Co., Ltd.


MIT : Miracle International Technology Co., Ltd.

This result calibrate was found accurate as shown on date place of calibrate only
This certificate is traceability to the International System of Unit (SI)

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k=2$, providing a level of confidence approximately 95%

Calibrated by : Mr. Thippatai Mungpungklang

Approved by :


Ms. Budsagorn Patcha
Authorized Signatory

This certificate may not be reproduced except in full unless permission for the reproduction has been obtained in writing from the laboratory.



Measuretronix Limited
2425/2 Lat Phrao Road, Saphan Song
Wangthonglang, Bangkok 10310, Thailand
Phone : 0-2514-1000, 0-2514-1234
Fax : 0-2514-0001, 0-2514-0003
Website : www.measuretronix.com



Certificate of Calibration

Certificate Number : LF25-0305
Equipment : Thermometer
Manufacturer : Fluke
Model : 51
Serial Number : 5910857
Asset Number : 5910857
Customer : Thai Unique Co., Ltd.
80-82 Prachathipatai Road,
Bangkhunphrom, Pranakorn,
Bangkok 10200
Date of Calibrate : 6-Jun-2025
Date of Issue : 6-Jun-2025

This calibration certificate documents the traceability to national standards, which realize the units of measurement according to the International System of Units (SI).

This calibration certificate applies only to the item identified and shall not be reproduced other than in full, without specific written approved by Measuretronix Cal-Lab. Calibration certificates without signature are not valid.

The measurements marked with an asterisk () in this certificate are outside our range of accreditation. They have been included for completeness.*

The Calibration interval (Cal.Due) is the responsibility of the end user.

Calibrated by

Samak

Mr. Samak Uaonkaonoi
Metrology Technician

Approved by

Miss Juthamas Sukhathainirun

Miss Juthamas Sukhathainirun
Cal-Lab Manager

Certificate No. : LF25-0305

Model : 51

Serial No. : 5910857

Page 1 of 3



Agilent Technologies

Certificate of Analysis

FID-TCID Performance Evaluation Sample Kit

Agilent Part
Number: 5080-8842, 18710-60170

Sample Lot
Number: 0006750304

This analytical reference material was manufactured and verified in accordance with an ISO 9001 registered quality system, and the analyte concentrations were verified by an ISO 17025 accredited laboratory. The certified value for each analyte was determined gravimetrically.

Concentrations:		
n-tetradecane	0.218 g/L ($\pm 0.5\%$)	0.033 w/w %
n-pentadecane	0.218 g/L ($\pm 0.5\%$)	0.033 w/w %
n-hexadecane	0.218 g/L ($\pm 0.5\%$)	0.033 w/w %


Solvent: hexane

Calibrated Class A glassware and clean bottles were used in the manufacture of this standard. Balances used in the manufacture of this standard are calibrated with weights traceable to NIST in compliance with ANSI/NCSL Z-540-1 and ISO 9001.

Purities:	
n-tetradecane	99.6%
n-pentadecane	99%
n-hexadecane	99.5%
hexane	99%

Typical Analytical Spectrum or Chromatography

GC Chromatography – n-tetradecane, n-pentadecane, and n-hexadecane in hexane

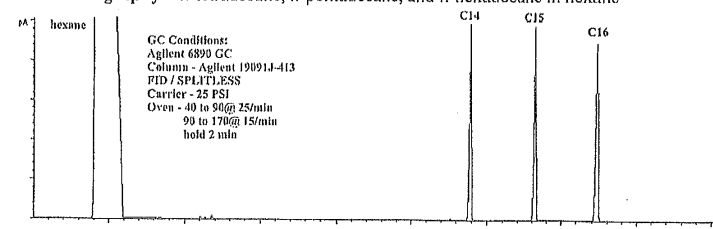

Date of release: 30 June 2023

Date of expiration: 31 July 2025

Monica Bourgeois
Monica Bourgeois
QMS Representative



CERTIFICATE No : 25M2254
REFERENCE No : 76365-1

PAGE : 1 OF 2

Certificate of Calibration

EQUIPMENT : DIGITAL BALANCE
MANUFACTURER : METTLER TOLEDO
MODEL : XS105DU
SERIAL No : 1126422905
ID No : BA05/50
CONDITION AS RECEIVED : USED ITEM
SUBMITTED BY : S.P.S. CONSULTING SERVICE CO., LTD.
7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN RD.,
JOMPOL, CHATUCHAK, BANGKOK 10900

CALIBRATED BY : ATSAWIN Y.
CALIBRATION DATE : 07-Mar-25

APPROVED BY : PONGSAK J.
ISSUED DATE : 13-Mar-25
RECEIVED DATE : 07-Mar-25

THIS CERTIFICATE MAY NOT BE REPRODUCED OTHER THAN IN FULL EXCEPT WITH THE PRIOR WRITTEN APPROVAL OF
QUALITY CALIBRATION CO., LTD.



CERTIFICATE No : 25M2254

PAGE : 2 OF 2

Calibration Report

EQUIPMENT : DIGITAL BALANCE MODEL : XS105DU
MANUFACTURER : METTLER TOLEDO S/N : 1126422905
ID No : BA05/50 RECEIVED DATE : 07-Mar-25
AIR PRESSURE : 1009mbar \pm 1mbar CALIBRATION DATE : 07-Mar-25
AMBIENT TEMPERATURE : 24°C \pm 1°C RELATIVE HUMIDITY : 54%RH \pm 10% RH

CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED BY ACCORDING TO UKAS LAB 14 EDITION 6:2019 BY USING KNOWN WEIGHT STANDARD WEIGHT. THE BALANCE WAS NOT ADJUSTED BEFORE CALIBRATION. THE BALANCE HAS NO ZERO TRACKING FUNCTION. REPEATABILITY WAS MEASURED BY USING 10 REPEATED MEASUREMENTS. LINEARITY WAS MEASURED COVERING 10 POINTS, EVENLY SPREAD OVER THE RANGE. THE INSTRUMENT WAS SET ZERO BEFORE PERFORMING THE LINEARITY TEST. OFF-CENTER LOADING WAS MEASURED BY USING STANDARD WEIGHTS PLACED ON THE PAN AND MOVED TO VARIOUS POSITIONS ON THE PAN.

2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) STANDARD WEIGHT SET	E2	QK-I-151	C02250116	28-Jan-27
2) STANDARD WEIGHT	E2	15843	C02250117	29-Jan-27

3. THE CERTIFICATE IS VALID FOR THE ITEM CALIBRATED AS SHOWN ON THE DATE AND PLACE OF CALIBRATION ONLY.

4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.

5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-
- NATIONAL INSTITUTE OF METROLOGY (THAILAND)

RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

- ZERO SETTING FUNCTION : NORMAL
- TARE FUNCTION : NORMAL
- REPEATABILITY OF READING AT 120 g WAS 0.000055 g
- DEPARTURE FROM NOMINAL VALUE/ LINEARITY

NOMINAL VALUE (g)	BALANCE READING (g)	CORRECTION (g)	UNCERTAINTY (\pm g)
0.00	0.00000	0.00000	0.000065
0.02	0.01999	0.00001	0.000065
0.10	0.10001	-0.00001	0.000066
0.20	0.20001	-0.00001	0.000066
0.50	0.50002	-0.00002	0.000065
1.00	1.00003	-0.00003	0.000066
2.00	2.00001	-0.00001	0.000067
5.00	5.00002	-0.00002	0.000068
10.00	10.00000	0.00000	0.000070
20.00	20.00004	-0.00004	0.000078
50.00	50.00000	0.00000	0.00013
100.00	100.0001	-0.0001	0.00019
120.00	120.0002	-0.0002	0.00022

5. OFF CENTER LOADING ERROR



POINT	READING (g)
1	50.0000
2	50.0000
3	50.0000
4	50.0000
5	50.0000
OFF-CENTER LOADING	0.0000

NOTE: THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA
THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR $k=2$, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT





Certificate of Calibration

Aquion : Anion (ID#894)

This certificate is to verify that instrument below are calibrated

by Archemica Lab Co.,Ltd.

AQUION S/N : 190840059

AS-DV S/N : 190915235

for

S.P.S. Consulting Service Co., Ltd.



บริษัท อาร์เคมีกา แล็บ จำกัด
ARCHEMICA LAB CO.,LTD.

Operator Signature : Teerapat B

Date : Jun 6, 2025

(Mr. Teerapat Boonla)

Application Chemist



WO-11540198/2025

MAINTENANCE AND TEST CERTIFICATE MODEL
OPTIMA 5300DV

Customer : <u>S.P.S.Consulting Service Co.,Ltd</u>	Date Tested: <u>July 1, 2025</u>
Address : <u>7 Soi Phaholyothin 24</u>	Recommendation Recertification
<u>Paholyothin Road</u>	Period <u>6</u> Months
Jompoi Chatuchak, Bangkok 1090	Recertification Due: <u>January 1, 2026</u>
User Name: <u>K.Phenpha Vipasthawatt</u>	Date Last Certified: <u>January 6, 2025</u>
Phone: <u>083-9269252</u>	Visit Number: <u>1of 2</u>
Fax: <u>02-513-4221</u>	PerkinElmer Phone: <u>02-719-6420 ext 206</u>
	PerkinElmer Fax: <u>02-318-5597</u>

CONFIGURATION TESTED		ACCESSORIES/COMPONENT NOT INCLUDED
MODEL	SERIAL NUMBER	
<u>OPTIMA 5300DV</u>	<u>077C7042401</u>	
TESTED EQUIPMENT	CALIBRATION NUMBER	EXPIRATION
<u>IPV Methods</u>		
TEST STANDARD USED	PART NUMBER	EXPIRATION DATE
<u>Multielement Standard</u>	<u>N069-1579</u>	<u>December 30, 2024</u>
<u>Wavecal Solution</u>	<u>N058-2152</u>	<u>March 30, 2024</u>
<u>VIS Wavecal solution</u>	<u>N930-2946</u>	<u>February 28, 2024</u>
<u>Instrument Cal. STD4</u>	<u>N930-0221</u>	<u>November 30, 2024</u>
CUSTOMER SUPPLIED	COMMENTS	CUSTOMER INITIALS
<u>2 % HNO3</u>		
<u>10 % HNO3</u>		

Page 1 of 4



WO-11540198/2025

MAINTENANCE AND TEST CERTIFICATE MODEL
OPTIMA 5300DV

SERIAL NUMBER <u>077C7042401</u>	DATE TESTED <u>July 1, 2025</u>
1. MECHANICAL CHECKS	
A. Inspect and clean all fans and filters.	<input type="checkbox"/> OK
B. Inspect and replace as necessary, all torch components including the RF coil.	<input type="checkbox"/> OK
C. Inspect all tubing for sign of clacking or leaking.	<input type="checkbox"/> OK
D. Adjust water and gas pressure regulator settings.	<input type="checkbox"/> OK
E. Inspect and leak check pneumatics drawers.	<input type="checkbox"/> OK
F. Clean the exterior of the instrument.	<input type="checkbox"/> OK
2. OPTICAL CHECKS	
A. Inspect and clean all optical components.	<input type="checkbox"/> OK
B. As required, check and replace all purgefilters.	<input type="checkbox"/> OK
C. Recheck optical alignment.	<input type="checkbox"/> OK
3. COOLING SYSTEM CHECKS	
A. Perform preventive maintenance on chiller.	<input type="checkbox"/> OK
B. Flush out the chiller every year.	<input type="checkbox"/> N/A
4. PERFORMANCE CHECKS	
A. Torch View Alignment.	<input type="checkbox"/> OK
B. Wavelength Calibration.	<input type="checkbox"/> OK

Page 2 of 4



MAINTENANCE AND TEST CERTIFICATE MODEL

OPTIMA 5300DV

SERIAL NUMBER : 077C7042401		DATE TESTED : July 1, 2025	
PARAMETER	SPECIFICATION		FINAL VALUE
Spectral Resolution : UV	As 193.696 nm	≤ 0.007	0.00570
	Ni 231.604 nm	≤ 0.008	0.00734
	Ni 341.476 nm	≤ 0.012	0.00763
Spectral Resolution : VIS	La 408.672 nm	≤ 0.020	0.01627
	Ba 455.403 nm	≤ 0.025	0.02428
Precision	As 193.656 nm	% RSD < 1.0	0.82 %
	Zn 213.856 nm	% RSD < 1.0	0.83 %
	Mn 257.610 nm	% RSD < 1.0	0.20 %
	La 379.478 nm	% RSD < 1.0	0.89 %
	Ba 455.403 nm	% RSD < 1.0	0.92 %
	Ba 493.408 nm	% RSD < 1.0	0.75 %
Detection Limits : Axial	Tl 190.080 nm	3(sd)	10.65 ppb
	As 193.696 nm	3(sd)	2.48 ppb
	Pb 220.353 nm	3(sd)	3.09 ppb
Detection Limits : Radial	As 193.696 nm	3(sd)	331.50 ppb
	Zn 213.856 nm	3(sd)	0.98 ppb
	Mn 257.610 nm	3(sd)	0.34 ppb
	La 379.478 nm	3(sd)	2.54 ppb
	Ba 455.403 nm	3(sd)	2.19 ppb
	Ba 493.408 nm	3(sd)	4.32 ppb
BEC : Axial (IB X 500)/(IS-IB)	Cd 226.502 nm	≤ 150 ppb	140.03
BEC : Radial (IB X 1000)/(IS-IB)	Mn 257.610 nm	≤ 45 ppb	24.17



MAINTENANCE AND TEST CERTIFICATE MODEL

OPTIMA 5300DV

SERIAL NUMBER	077C7042401	DATE TESTED	July 1, 2025
---------------	-------------	-------------	--------------

Remarks :

Commissioning follow as commissioning performance sheets.

This is to certify that the above tests have been performed and the configuration tested

☒ meets
☐ does not meet

the PerkinElmer Specifications listed on this certificate.

This certificate does not modify PerkinElmer's standard terms and condition of sale, including warranty terms.

Service Department PerkinElmer Ltd.

Authorized Representative: *Wiphan Promlumda*

(Wiphan Promlumda)
Service Engineer

เอกสารแนบ 5-7

เอกสารสอบเทียบเครื่องมือการตรวจวัดระดับเสียงในสถานประกอบการ



THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-68/0220

MTC No. EEL. BP. 44/0268

CALIBRATION CERTIFICATE

Submitted by : S.P.S.Consulting Service Co.,Ltd.

Address : 7 Soi Phaholyothin 24, Phaholyothin Road, Jompol, Chatuchak, Bangkok 10900.

Calibrated at : Electrical and Electronic Standards Laboratory, Industrial Metrology and Testing Service Centre.
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Rd., Muang, Samutprakan 10280.

Instrument Calibrated :

Description : Sound Calibrator

Manufacturer : ACO

Model : 2127

Serial No. : 130006

Ambient Environment

Temperature : (23 ± 3) °C

Relative Humidity : (50 ± 15) %

Ambient Pressure : (101.325 ± 1.500) kPa

- Standards used :
1. Digital Function Synthesizer NF Electronic DF-193A S/N 122037.
 2. Measuring Amplifier Bruel&Kjaer 2636 S/N 1537484.
 3. Programmable Attenuator Tamagawa TPA-303A S/N OF 2214.
 4. Digital Multimeter Agilent 34401A S/N MY44005560.
 5. Pressure Transmitter Vaisala PTB202AD S/N T0650001.
 6. Audio Analyzer Panasonic VP-7722A S/N 041477D122.
 7. Condenser Microphone B&K 4180 S/N 2889871.

Calibration Procedure: CP-102-04 based on IEC 60942-2003; The sound pressure level generated by sound calibrator under test shall be measured by standard microphone using an insert voltage technique.

This instrument has been calibrated against standards maintained at Electrical and Electronic Standards Laboratory (EEL), which are traceable to the International System of Units through the National Institute of Metrology (Thailand).

The information on actual reading is attached herewith and the uncertainty limits quoted refer to the measured values only.

Date of Receipt : 19 Feb. 2025

Date of Calibration : 21 Feb. 2025

1 / 2

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BLMTC.002 Rev.5



THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-68/0220

MTC No. EEL. BP. 44/0268

The reported expanded uncertainty is based upon a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%.

Nominal Output of Unit Under Test = 94 dB re 20μPa at 1000 Hz

Acoustic Output in dB re 20μPa, Corrected to Reference Conditions: 101.325 kPa, 23.0 °C and 50 %RH.

1. Sound Pressure Level

Standard Microphone Type	Measured Sound Pressure Level (dB)	Deviated value (dB)	Uncertainty (dB)	Tolerance limit IEC60942:2003 Class 1
1/2 inch Bruel&Kjaer 4180	93.81	-0.19	± 0.10	±0.40 dB

2. Frequency

Standard Microphone Type	Measured Frequency (Hz)	Deviated value (Hz)	Uncertainty (Hz)	Tolerance limit IEC60942:2003 Class 1
1/2 inch Bruel&Kjaer 4180	999.9	-0.1	± 1.5	±1.0%

3. Total Distortion

Standard Microphone Type	Measured Total Distortion (%)	Uncertainty (%)	Tolerance limit IEC60942:2003 Class 1
1/2 inch Bruel&Kjaer 4180	0.95	± 0.50	±3.0%

Note : 1. No adjustment.

2. The calibrator pressure correction was not included.

3. The microphone volume correction was not included.

Calibrated by :

Mr. Weerachai Deechaiyae
(Mr. Weerachai Deechaiyae)

Approved by :

Mr. Prawate Kluaypa
Director
Electrical and Electronic Standards Laboratory

Date of Calibration : 21 Feb. 2025

Date of Issue : 24 Feb. 2025

Industrial Metrology and Testing Service Centre

Ref : 2011268021900739001

End of Certificate

2 / 2

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BLMTC.002 Rev.5

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9009

Office/Laboratory
668 Mu 2 Tambon Bangpoornai, Amphoe Muang Samutprakan,
Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtc@tistr.or.th Website : www.tistr.or.th

Office
196 Phahonyothin Road, Ladyao, Chatuchak,
Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9009

Office/Laboratory
668 Mu 2 Tambon Bangpoornai, Amphoe Muang Samutprakan,
Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtc@tistr.or.th Website : www.tistr.or.th

Office
196 Phahonyothin Road, Ladyao, Chatuchak,
Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด

S.P.S. CONSULTING SERVICE CO., LTD.

7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900

7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900

Tel : (662) 939-4370-72 Fax : (662) 513-4221 E-mail : sale@spscon.com, www.spscon.com

Noise R_554/25

Sound Level Meter Calibration Report


Acoustic Calibrator Data

Brand	ACO	Number	AC 03/56
Model	2127	Serial No.	130006
Calibration Range	94 dB, 1000 Hz	Last Calibration	21 February 2025
		Due Date	21 February 2026

Calibration Data

Sound Level Meter Data				Calibration Data		
SLM No.	Brand	Model	Serial No.	Date	Actual Reading [dB]	
					Before Adjustment	After Adjustment
ACO-R40	ACO	6236	00192052	30 September 2025	93.9	93.9
ACO-R41	ACO	6236	00192053	30 September 2025	93.9	93.9
ACO-R50	ACO	6236	00192062	30 September 2025	93.9	93.9
ACO-R51	ACO	6236	00192063	30 September 2025	93.9	93.9
Acoustic Certified Value : Thailand Institute of Scientific and Technological Research (TISTR)					93.81 ± 0.10 dB	

Calibrated by : Adul Dangklom
(Mr. Adul Dangklom)

Approved by : 
(Mr. Peera Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

Noise R_587/25

Sound Level Meter Calibration Report

Acoustic Calibrator Data

Brand	ACO	Number	AC 03/56
Model	2127	Serial No.	130006
Calibration Range	94 dB, 1000 Hz	Last Calibration	21 February 2025
		Due Date	21 February 2026

Calibration Data

Sound Level Meter Data					Calibration Data	
SLM No.	Brand	Model	Serial No.	Date	Actual Reading [dB]	
					Before Adjustment	After Adjustment
ACO-R52	ACO	6236	19206446	16 October 2025	93.9	93.9
Acoustic Certified Value : Thailand Institute of Scientific and Technological Research (TISTR)					93.81 ± 0.10 dB	

Calibrated by :

Adul Dangklom
(Mr. Adul Dangklom)

Approved by :

Peera Detudom
(Mr. Peera Detudom)

เอกสารแนบ 5-8

เอกสารสอบเทียบเครื่องมือการตรวจวัดปริมาณเสียงสะสมติดตัวพนักงาน



THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-67/0562

MTC No. EEL. BP. 71/0767

CALIBRATION CERTIFICATE

Submitted by : S.P.S Consulting Services Co.,Ltd.

Address : 7 Soi Phaholyothin 24, Phaholyothin Road, Jompol, Chatuchak, Bangkok 10900.

Calibrated at : Electrical and Electronic Standards Laboratory, Industrial Metrology and Testing Service Centre.
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Rd., Muang, Samutprakan 10280.

Instrument Calibrated :

Description : Sound Calibrator

Manufacturer : SVANTEK

Model : SV34

Serial No. : 33137

Standards used : 1. Digital Function Synthesizer NF Electronic DF-193A S/N 122037.

2. Measuring Amplifier Bruel&Kjaer 2636 S/N 1537484.

3. Programmable Attenuator Tamagawa TPA-303A S/N OF 2214.

4. Digital Multimeter Agilent 34401A S/N MY44005560.

5. Pressure Transmitter Vaisala PTB202AD S/N T0650001.

6. Audio Analyzer Panasonic VP-7722A S/N 041477D122.

7. Condenser Microphone Bruel&Kjaer 4180 S/N 2633526.

Ambient Environment

Temperature : $(23 \pm 3) ^\circ\text{C}$

Relative Humidity : $(50 \pm 15) \%$

Ambient Pressure : $(101.325 \pm 1.500) \text{ kPa}$

Calibration Procedure: CP-102-04 based on IEC 60942-2003; The sound pressure level generated by sound calibrator under test shall be measured by standard microphone using an insert voltage technique.

This instrument has been calibrated against standards maintained at Electrical and Electronic Standards Laboratory (EEL), which are traceable to the International System of Units through the National Institute of Metrology (Thailand).

The information on actual reading is attached herewith and the uncertainty limits quoted refer to the measured values only.

Date of Receipt : 31 Jul. 2024

Date of Calibration : 6 Aug. 2024

1/2

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BLMTC.002 Rev.5



THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-67/0562

MTC No. EEL. BP. 71/0767

The reported expanded uncertainty is based upon a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%.

Nominal Output of Unit Under Test = 114 dB re 20 μPa at 1000 Hz

Acoustic Output in dB re 20 μPa , Corrected to Reference Conditions: 101.325 kPa, 23.0 $^\circ\text{C}$ and 50 %RH.

1. Sound Pressure Level

Standard Microphone Type	Measured Sound Pressure Level (dB)	Deviated value (dB)	Uncertainty (dB)	Tolerance limit IEC60942:2003 Class 2
1/2 inch Bruel&Kjaer 4180	113.50	-0.50	± 0.10	$\pm 0.75 \text{ dB}$

2. Frequency

Standard Microphone Type	Measured Frequency (Hz)	Deviated value (Hz)	Uncertainty (Hz)	Tolerance limit IEC60942:2003 Class 2
1/2 inch Bruel&Kjaer 4180	1000.0	0.0	± 1.5	$\pm 2.0\%$

3. Total Distortion

Standard Microphone Type	Measured Total Distortion (%)	Uncertainty (%)	Tolerance limit IEC60942:2003 Class 2
1/2 inch Bruel&Kjaer 4180	0.48	± 0.50	$\pm 4.0\%$

Note : 1. No adjustment.

2. The calibrator pressure correction was not included.

3. The microphone volume correction was not included.

Calibrated by :

(Mr. Weerachai Deechaiyae)

Approved by :

(Mr. Prawate Kluaypa)

Director

Electrical and Electronic Standards Laboratory

Industrial Metrology and Testing Service Centre

Date of Calibration : 6 Aug. 2024

Date of Issue : 7 Aug. 2024

Ref : 2011267073102836002

End of Certificate

2 / 2

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BLMTC.002 Rev.5

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9009

Office/Laboratory
668 Mu 2 Tambon Bangpoomai, Amphoe Muang Samutprakan,
Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtc@tistr.or.th Website : www.tistr.or.th

Office
196 Phahonyothin Road, Ladyao, Chatuchak,
Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9009

Office/Laboratory
668 Mu 2 Tambon Bangpoomai, Amphoe Muang Samutprakan,
Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtc@tistr.or.th Website : www.tistr.or.th

Office
196 Phahonyothin Road, Ladyao, Chatuchak,
Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827

Noise Dose R_270/25

Noise Dose Meter Calibration Report

Acoustic Calibrator Data

Brand	SVANTEK	Number	SV 01/60
Model	SV34	Serial No.	33137
Calibration Range	114 dB, 1000 Hz	Last Calibration	06 August 2024
		Due Date	06 August 2025

Calibration Data

Sound Level Meter Data

Calibration Data

SLM No.	Brand	Model	Serial No.	Date	Actual Reading [dB]	
					Before Adjustment	After Adjustment
NMD-B15	SVANTEK	SV-104IS	80880	27 April 2025	113.5	113.5
NMD-R03	SVANTEK	SV-104IS	60153	27 April 2025	113.5	113.5
NMD-R22	SVANTEK	SV-104IS	80801	27 April 2025	113.6	113.5
NMD-R26	SVANTEK	SV-104IS	80836	27 April 2025	113.5	113.5
NMD-R35	SVANTEK	SV-104IS	80873	27 April 2025	113.5	113.5
Acoustic Certified Value : Thailand Institute of Scientific and Technological Research (TISTR)					113.50± 0.10 dB	

Calibrated by : Adul Dangklom
(Mr. Adul Dangklom)

Approved by : Peera Detudom
(Mr. Peera Detudom)

Noise Dose R_270-1/25

Noise Dose Meter Calibration Report

Acoustic Calibrator Data

Brand	SVANTEK	Number	SV 01/60
Model	SV34	Serial No.	33137
Calibration Range	114 dB, 1000 Hz	Last Calibration	06 August 2024
		Due Date	06 August 2025

Calibration Data

Sound Level Meter Data

Calibration Data

SLM No.	Brand	Model	Serial No.	Date	Actual Reading [dB]	
					Before Adjustment	After Adjustment
NMD-R22	SVANTEK	SV-104IS	80801	06 May 2025	113.6	113.5
NMD-R26	SVANTEK	SV-104IS	80836	06 May 2025	113.5	113.5
NMD-R35	SVANTEK	SV-104IS	80873	06 May 2025	113.5	113.5
Acoustic Certified Value : Thailand Institute of Scientific and Technological Research (TISTR)					113.50± 0.10 dB	

Calibrated by : Adul Dangklom
(Mr. Adul Dangklom)

Approved by : Peera Detudom
(Mr. Peera Detudom)


Noise Dose R_326/25

Noise Dose Meter Calibration Report

Acoustic Calibrator Data						
Brand	SVANTEK		Number	SV 01/60		
Model	SV34		Serial No.	33137		
Calibration Range	114 dB, 1000 Hz		Last Calibration	06 August 2024		
			Due Date	06 August 2025		

Calibration Data						
Sound Level Meter Data				Calibration Data		
SLM No.	Brand	Model	Serial No.	Date	Actual Reading [dB]	
					Before Adjustment	After Adjustment
NMD-R26	SVANTEK	SV-104IS	80836	25 May 2025	113.5	113.5
NMD-R35	SVANTEK	SV-104IS	80873	25 May 2025	113.5	113.5
Acoustic Certified Value : Thailand Institute of Scientific and Technological Research (TISTR)					113.50± 0.10 dB	

Calibrated by : Adul Dangklom
 (Mr. Adul Dangklom)

Approved by : 
 (Mr. Peera Detudom)

เอกสารแนบ 5-9

เอกสารสอบเทียบเครื่องมือการตรวจวัดแสงสว่างในสถานประกอบการ



Certificate of Calibration

Certificate Number : SPR25080318-1 Page : 1 of 3
 Customer : S.P.S. CONSULTING SERVICE CO., LTD.
 7 Soi Phaholyothin 24 Phaholyothin Road., Jompol, Chatuchak,
 Bangkok 10900

Equipment Name : Light Meter
 Manufacturer : Extech
 Model : 407026
 Serial Number : A.052323
 ID. Number : LUX- R07

Environmental Conditions

Ambient Temperature : 23 °C ± 3 °C Received Date : 19 Aug 2025
 Relative Humidity : 50 % ± 15 % Calibration Date : 22 Aug 2025
 Location of Calibration : In-Lab Recommend Due Date : 22 Aug 2026
 Calibration Procedure : SP-CPE-04-32 Date of Issue : 23 Aug 2025

Method of Calibration

This certifies that the above instrument was calibrated in compliance with the calibration system requirement of ISO/IEC 17025:2017 in accordance with reference procedure. Standards used to perform this calibration are certified by to NIST or equivalent, National metrology institute, Natural physical constants, consensus standards. The result reported herein apply only to the calibration of the item described above as received. Our decision rule is to contact the customer if the item pass and fail calibration when the results include the uncertainties and the customer must determine if the results meets their needs. The calibration certificate shall not be reproduced except in full, without written approval of SP Metrology System (Thailand).

Calibrated by : Mr.Chumpon Dokpikul

Calibration Officer

Approved by

(Mr.Pootthipong A.)

Authorized Signatory



SP-FM-04-15 rev.0



Calibration Report

Certificate Number : SPR25080318-1 Page : 2 of 3

Reference Standards

Equipment Name	Model	Serial No.	Certificate No.	Due. Date
Digital Light Meter	LX-73	Q842777	24PH432	21 Aug 2026

Traceability

This certification is traceable to the International System of Unit maintained at :
 TPA - Technology Promotion Association (Thailand-Japan)

SP-FM-04-15 rev.0

69/29 Moo 1 Klongsi Klongluang Pathumthani 12120 Tel: (662) 193-2217-20 www.spmetrology.co.th

69/29 Moo 1 Klongsi Klongluang Pathumthani 12120 Tel: (662) 193-2217-20 www.spmetrology.co.th



Result of Calibration

Certificate Number : SPR25080318-1

Page : 3 of 3

Function: Illumination Measurement

Unit : Lux

Calibration Point	Standard Reading	UUC Reading	Error	Uncertainty (±)
100	100.0	100	0	1.7
200	200	201	1	6.6
300	300	302	2	6.6
1000	1000	997	-3	13
2000	2000	1990	-10	26
3000	3000	2980	-20	39

Note :

The result of calibration was found accurate as show on date and place of calibration only.
This Certificate is not certified for any commercial transaction.

Measurement Uncertainty

The reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor $k = 2.00$, providing a level of confidence approximately 95 %

- End of Certificate -

เอกสารแนบ 5-10

เอกสารสอบเทียบเครื่องมือการตรวจวัดระดับความร้อนในสถานประกอบการ



ID LINE : IEC17025



Certificate of Calibration

Certificate Number : SPR25030358-6

Page : 1 of 3

Customer : S.P.S. CONSULTING SERVICE CO., LTD.

7 Soi Phaholyothin 24 Phaholyothin Road., Jompol, Chatuchak,
Bangkok 10900

Equipment Name : Area Heat Stress Monitor

Manufacturer : Metrosonics

Model : hs-32

Serial Number : MCE030011

ID. Number : B21

Environmental Conditions

Ambient Temperature : 23 °C ± 2 °C

Relative Humidity : 50 % ± 15 %

Location of Calibration : In-Lab

Calibration Procedure : SP-CPT-04-13

Received Date : 19 Mar 2025

Calibration Date : 27 Mar 2025

Recommend Due Date : 27 Mar 2026

Date of Issue : 28 Mar 2025

Method of Calibration


This certifies that the above instrument was calibrated in compliance with the calibration system requirement of ISO/IEC 17025:2017 in accordance with reference procedure. Standards used to perform this calibration are certified by to NIST or equivalent, National metrology institute, Natural physical constants, consensus standards. The result reported herein apply only to the calibration of the item described above as received. Our decision rule is to contact the customer if the item pass and fail calibration when the results include the uncertainties and the customer must determine if the results meets their needs.

The calibration certificate shall not be reproduced except in full, without written approval of SP Metrology System (Thailand).

Calibrated by : Mr.Surasak Ritthikaew

Calibration Officer

Approved by :


(Mr.Prayoon Topart)

Authorized Signatory



ID LINE : IEC17025



Calibration Report

Certificate Number : SPR25030358-6

Page : 2 of 3

Reference Standards

Equipment Name	Model	Serial No.	Certificate No.	Due. Date
Humidity Chamber	TH-80S	N/A	SPR25010173-14	30 Jan 2026
THERMO-HYGROMETER	5020A	A47046	TMU2500342	29 Jan 2026

Traceability

This certification is traceable to the International System of Unit maintained at :

SP Metrology - SP Metrology system (Thailand) Co.Ltd.

NA - NA Caltechnologies Co., Ltd.



Result of Calibration

Certificate Number : SPR25030358-6

Page : 3 of 3

Temperature Accuracy in the Measurement. (WET)

Unit : °C

Temperature Setting	Standard Reading	UUC Reading	Error	Uncertainty (±)
30.0	29.985	29.8	-0.185	0.20
35.0	34.988	34.8	-0.188	0.20
40.0	39.990	39.9	-0.090	0.20

Temperature Accuracy in the Measurement. (DRY)

Unit : °C

Temperature Setting	Standard Reading	UUC Reading	Error	Uncertainty (±)
30.0	29.985	29.7	-0.285	0.20
35.0	34.988	34.7	-0.288	0.20
40.0	39.990	39.8	-0.190	0.20

Temperature Accuracy in the Measurement. (GLOBE)

Unit : °C

Humidity Setting	Standard Reading	UUC Reading	Error	Uncertainty (±)
30.0	29.985	29.7	-0.285	0.20
35.0	34.988	34.7	-0.288	0.20
40.0	39.990	39.7	-0.290	0.20

Note :

The result of calibration was found accurate as show on date and place of calibration only.
This Certificate is not certified for any commercial transaction.

Measurement Uncertainty

The reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor $k = 2$, providing a level of confidence approximately 95%.

- End of Certificate -

Certificate of Calibration

Certificate Number : SPR25030358-2 Page : 1 of 3

Customer : S.P.S. CONSULTING SERVICE CO., LTD.
7 Soi Phaholyothin 24 Phaholyothin Road., Jompol, Chatuchak,
Bangkok 10900

Equipment Name : Area Heat Stress Monitor

Manufacturer : Quest Technologies

Model : QUESTemp 32

Serial Number : TPH050015

ID. Number : B32

Environmental Conditions

Ambient Temperature	: 23 °C ± 2 °C	Received Date	: 19 Mar 2025
Relative Humidity	: 50 % ± 15 %	Calibration Date	: 22 Mar 2025
Location of Calibration	: In-Lab	Recommend Due Date	: 22 Mar 2026
Calibration Procedure	: SP-CPT-04-13	Date of Issue	: 23 Mar 2025

Method of Calibration

This certifies that the above instrument was calibrated in compliance with the calibration system requirement of ISO/IEC 17025:2017 in accordance with reference procedure. Standards used to perform this calibration are certified by to NIST or equivalent, National metrology institute, Natural physical constants, consensus standards. The result reported herein apply only to the calibration of the item described above as received. Our decision rule is to contact the customer if the item pass and fail calibration when the results include the uncertainties and the customer must determine if the results meets their needs.

The calibration certificate shall not be reproduced except in full, without written approval of SP Metrology System (Thailand).

Calibrated by : Mr. Navaporn Uengseng

Calibration Officer

Approved by : 

(Mr. Pootthipong A.)

Authorized Signatory

Calibration Report

Certificate Number : SPR25030358-2 Page : 2 of 3

Reference Standards

Equipment Name	Model	Serial No.	Certificate No.	Due. Date
Humidity Chamber	TH-80S	N/A	SPR25010173-14	30 Jan 2026
THERMO-HYGROMETER	5020A	A47046	TMU2500342	29 Jan 2026

Traceability

This certification is traceable to the International System of Unit maintained at :

SP Metrology - SP Metrology system (Thailand) Co.Ltd.

NA - NA Caltechnologies Co., Ltd.

Result of Calibration



ID LINE : IEC17025

Certificate Number : SPR25030358-2

Page : 3 of 3

Temperature Accuracy in the Measurement. (WET)

Unit : °C

Temperature Setting	Standard Reading	UUC Reading	Error	Uncertainty (±)
30.0	30.015	29.9	-0.115	0.20
35.0	35.012	34.9	-0.112	0.20
40.0	40.016	39.9	-0.116	0.20

Temperature Accuracy in the Measurement. (DRY)

Unit : °C

Temperature Setting	Standard Reading	UUC Reading	Error	Uncertainty (±)
30.0	30.015	30.0	-0.015	0.20
35.0	35.012	35.0	-0.012	0.20
40.0	40.016	40.0	-0.016	0.20

Temperature Accuracy in the Measurement. (GLOBE)

Unit : °C

Temperature Setting	Standard Reading	UUC Reading	Error	Uncertainty (±)
30.0	30.015	30.2	0.185	0.20
35.0	35.012	35.2	0.188	0.20
40.0	40.016	40.2	0.184	0.20

Note:

The result of calibration was found accurate as show on date and place of calibration only.
This Certificate is not certified for any commercial transaction.

Measurement Uncertainty

The reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor $k = 2$, providing a level of confidence approximately 95%.

- End of Certificate -



ID LINE : IEC17025



Certificate of Calibration

Certificate Number : SPR25030358-4

Page : 1 of 3

Customer : S.P.S. CONSULTING SERVICE CO., LTD.

7 Soi Phaholyothin 24 Phaholyothin Road., Jompol, Chatuchak,
Bangkok 10900

Equipment Name : Area Heat Stress Monitor

Manufacturer : Metrosonics

Model : hs-32

Serial Number : MCD070035

ID. Number : R05

Environmental Conditions

Ambient Temperature : 23 °C ± 2 °C

Relative Humidity : 50 % ± 15 %

Location of Calibration : In-Lab

Calibration Procedure : SP-CPT-04-13

Received Date : 19 Mar 2025

Calibration Date : 27 Mar 2025

Recommend Due Date : 27 Mar 2026

Date of Issue : 28 Mar 2025

Method of Calibration

This certifies that the above instrument was calibrated in compliance with the calibration system requirement of ISO/IEC 17025:2017 in accordance with reference procedure. Standards used to perform this calibration are certified by to NIST or equivalent, National metrology institute, Natural physical constants, consensus standards. The result reported herein apply only to the calibration of the item described above as received. Our decision rule is to contact the customer if the item pass and fail calibration when the results include the uncertainties and the customer must determine if the results meets their needs.

The calibration certificate shall not be reproduced except in full, without written approval of SP Metrology System (Thailand).

Calibrated by : Mr.Surasak Ritthikaew

Calibration Officer

Approved by :

(Mr.Prayodn Topart)

Authorized Signatory



ID LINE : IEC17025



Calibration Report

Certificate Number : SPR25030358-4

Page : 2 of 3

Reference Standards

Equipment Name	Model	Serial No.	Certificate No.	Due. Date
Humidity Chamber	TH-80S	N/A	SPR25010173-14	30 Jan 2026
THERMO-HYGROMETER	5020A	A47046	TMU2500342	29 Jan 2026

Traceability

This certification is traceable to the International System of Unit maintained at :
SP Metrology - SP Metrology system (Thailand) Co.Ltd.

NA - NA Caltechnologies Co., Ltd.



Result of Calibration

Certificate Number : SPR25030358-4

Page : 3 of 3

Temperature Accuracy in the Measurement. (WET)

Unit : °C

Temperature Setting	Standard Reading	UUC Reading	Error	Uncertainty (±)
30.0	29.987	29.8	-0.187	0.20
35.0	34.982	34.8	-0.182	0.20
40.0	39.990	39.8	-0.190	0.20

Temperature Accuracy in the Measurement. (DRY)

Unit : °C

Temperature Setting	Standard Reading	UUC Reading	Error	Uncertainty (±)
30.0	29.987	29.8	-0.187	0.20
35.0	34.982	34.8	-0.182	0.20
40.0	39.990	39.8	-0.190	0.20

Temperature Accuracy in the Measurement. (GLOBE)

Unit : °C

Humidity Setting	Standard Reading	UUC Reading	Error	Uncertainty (±)
30.0	29.987	29.7	-0.287	0.20
35.0	34.982	34.8	-0.182	0.20
40.0	39.990	39.8	-0.190	0.20

Note :

The result of calibration was found accurate as show on date and place of calibration only.

This Certificate is not certified for any commercial transaction.

Measurement Uncertainty

The reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor $k = 2$, providing a level of confidence approximately 95%.

- End of Certificate -



ID LINE : IEC17025



Certificate of Calibration

Certificate Number : SPR25030358-5

Page : 1 of 3

Customer : S.P.S. CONSULTING SERVICE CO., LTD.

7 Soi Phaholyothin 24 Phaholyothin Road., Jompol, Chatuchak,
Bangkok 10900

Equipment Name : Area Heat Stress Monitor

Manufacturer : Quest Technologies

Model : QUESTemp 34

Serial Number : TEH090208

ID. Number : R08

Environmental Conditions

Ambient Temperature : 23 °C ± 2 °C

Relative Humidity : 50 % ± 15 %

Location of Calibration : In-Lab

Calibration Procedure : SP-CPT-04-13

Received Date : 19 Mar 2025

Calibration Date : 27 Mar 2025

Recommend Due Date : 27 Mar 2026

Date of Issue : 28 Mar 2025

Method of Calibration


This certifies that the above instrument was calibrated in compliance with the calibration system requirement of ISO/IEC 17025:2017 in accordance with reference procedure. Standards used to perform this calibration are certified by to NIST or equivalent, National metrology institute, Natural physical constants, consensus standards. The result reported herein apply only to the calibration of the item described above as received. Our decision rule is to contact the customer if the item pass and fail calibration when the results include the uncertainties and the customer must determine if the results meets their needs.

The calibration certificate shall not be reproduced except in full, without written approval of SP Metrology System (Thailand).

Calibrated by : Mr.Surasak Ritthikaew

Calibration Officer

Approved by :


(Mr.Prayoon Topart)

Authorized Signatory



ID LINE : IEC17025



Calibration Report

Certificate Number : SPR25030358-5

Page : 2 of 3

Reference Standards

Equipment Name	Model	Serial No.	Certificate No.	Due. Date
Humidity Chamber	TH-80S	N/A	SPR25010173-14	30 Jan 2026
THERMO-HYGROMETER	5020A	A47046	TMU2500342	29 Jan 2026

Traceability

This certification is traceable to the International System of Unit maintained at :

SP Metrology - SP Metrology system (Thailand) Co.Ltd.

NA - NA Caltechnologies Co., Ltd.



ID LINE : IEC17025



Result of Calibration

Certificate Number : SPR25030358-5

Page : 3 of 3

Temperature Accuracy in the Measurement. (WET)

Unit : °C

Temperature Setting	Standard Reading	UUC Reading	Error	Uncertainty (±)
30.0	29.995	29.8	-0.195	0.20
35.0	34.990	34.8	-0.190	0.20
40.0	39.985	39.8	-0.185	0.20

Temperature Accuracy in the Measurement. (DRY)

Unit : °C

Temperature Setting	Standard Reading	UUC Reading	Error	Uncertainty (±)
30.0	29.995	29.7	-0.295	0.20
35.0	34.990	34.7	-0.290	0.20
40.0	39.985	39.7	-0.285	0.20

Temperature Accuracy in the Measurement. (GLOBE)

Unit : °C

Humidity Setting	Standard Reading	UUC Reading	Error	Uncertainty (±)
30.0	29.995	29.8	-0.195	0.20
35.0	34.990	34.8	-0.190	0.20
40.0	39.985	39.8	-0.185	0.20

Note :

The result of calibration was found accurate as show on date and place of calibration only.
This Certificate is not certified for any commercial transaction.

Measurement Uncertainty

The reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor $k = 2$, providing a level of confidence approximately 95%.

- End of Certificate -



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72. Fax : (662) 513-4221. E-mail : sale@spscon.com., www.spscon.com

Heat R092

Heat Stress WBGT Meter Verification Report			
Verification Data			
Heat Stress WBGT Meter No.	: B21	Verification Date	: 30 September 2025
Brand	: METROSNIcs	Ambient Temp.	: 24.5 °C
Model	: hs-32	Barometric Pressure	: 1011 mmbar
Serial No.	: MCE030011	Relative Humidity	: 49 %
Verification Module (Electronic Sensor Check) :			
Verification Module No. : 21 WB = 12.5 °C, DB = 47.1 °C, G = 69.3 °C			
Result of Verification : Without Adjustment			
Wet Probe Temperature Measurement			
Verification Module Reading (°C)	UUC* Reading (°C)	Correction (°C)	Tolerance Limit (°C)
12.5	12.6	-0.1	± 0.5
Dry Probe Temperature Measurement			
Verification Module Reading (°C)	UUC* Reading (°C)	Correction (°C)	Tolerance Limit (°C)
47.1	47.2	-0.1	± 0.5
Globe Probe Temperature Measurement			
Verification Module Reading (°C)	UUC* Reading (°C)	Correction (°C)	Tolerance Limit (°C)
69.3	69.2	0.1	± 0.5
UUC* = UNIT UNDER CALIBRATION			

Verified by : Adul Dangklom
(Mr.Adul Dangklom)

Approved by : 
(Mr. Peera Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72. Fax : (662) 513-4221. E-mail : sale@spscon.com., www.spscon.com

Heat R092

Heat Stress WBGT Meter Verification Report			
Verification Data			
Heat Stress WBGT Meter No.	: B32	Verification Date	: 30 September 2025
Brand	: Quest Technologies	Ambient Temp.	: 24.5 °C
Model	: QUESTemp ^o 32	Barometric Pressure	: 1011 mmbar
Serial No.	: TPH050015	Relative Humidity	: 49 %
Verification Module (Electronic Sensor Check) :			
Verification Module No. : 21 WB = 12.5 °C, DB = 47.1 °C, G = 69.3 °C			
Result of Verification : Without Adjustment			
Wet Probe Temperature Measurement			
Verification Module Reading (°C)	UUC* Reading (°C)	Correction (°C)	Tolerance Limit (°C)
12.5	12.6	-0.1	± 0.5
Dry Probe Temperature Measurement			
Verification Module Reading (°C)	UUC* Reading (°C)	Correction (°C)	Tolerance Limit (°C)
47.1	47.2	-0.1	± 0.5
Globe Probe Temperature Measurement			
Verification Module Reading (°C)	UUC* Reading (°C)	Correction (°C)	Tolerance Limit (°C)
69.3	69.2	0.1	± 0.5
UUC* = UNIT UNDER CALIBRATION			

Verified by : Adul Dangklom
(Mr.Adul Dangklom)

Approved by : 
(Mr. Peera Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

Heat R092

Heat Stress WBGT Meter Verification Report			
Verification Data			
Heat Stress WBGT Meter No. :	R05	Verification Date :	30 September 2025
Brand :	METROSONICS	Ambient Temp. :	24.5 °C
Model :	hs-32	Barometric Pressure :	1011 mmbar
Serial No. :	MCD070035	Relative Humidity :	49 %
Verification Module (Electronic Sensor Check) :			
Verification Module No. : 21 WB = 12.5 °C, DB = 47.1 °C, G = 69.3 °C			
Result of Verification : Without Adjustment			
Wet Probe Temperature Measurement			
Verification Module Reading (°C)	UUC* Reading (°C)	Correction (°C)	Tolerance Limit (°C)
12.5	12.7	-0.2	± 0.5
Dry Probe Temperature Measurement			
Verification Module Reading (°C)	UUC* Reading (°C)	Correction (°C)	Tolerance Limit (°C)
47.1	47.0	0.1	± 0.5
Globe Probe Temperature Measurement			
Verification Module Reading (°C)	UUC* Reading (°C)	Correction (°C)	Tolerance Limit (°C)
69.3	69.3	0.0	± 0.5
UUC* = UNIT UNDER CALIBRATION			

Verified by : Adul Dangklom
(Mr.Adul Dangklom)

Approved by : (Signature)
(Mr. Peera Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

Heat R092

Heat Stress WBGT Meter Verification Report			
Verification Data			
Heat Stress WBGT Meter No. :	R08	Verification Date :	30 September 2025
Brand :	Quest Technologies	Ambient Temp. :	24.5 °C
Model :	QUESTemp 34	Barometric Pressure :	1011 mmbar
Serial No. :	TEH090208	Relative Humidity :	49 %
Verification Module (Electronic Sensor Check) :			
Verification Module No. : 21 WB = 12.5 °C, DB = 47.1 °C, G = 69.3 °C			
Result of Verification : Without Adjustment			
Wet Probe Temperature Measurement			
Verification Module Reading (°C)	UUC* Reading (°C)	Correction (°C)	Tolerance Limit (°C)
12.5	12.4	0.1	± 0.5
Dry Probe Temperature Measurement			
Verification Module Reading (°C)	UUC* Reading (°C)	Correction (°C)	Tolerance Limit (°C)
47.1	47.3	-0.2	± 0.5
Globe Probe Temperature Measurement			
Verification Module Reading (°C)	UUC* Reading (°C)	Correction (°C)	Tolerance Limit (°C)
69.3	69.3	0.0	± 0.5
UUC* = UNIT UNDER CALIBRATION			

Verified by : Adul Dangklom
(Mr.Adul Dangklom)

Approved by : (Signature)
(Mr. Peera Detudom)