

ภาคผนวก จ



เอกสารเทียบเครื่องมือที่ใช้ในการตรวจวิเคราะห์

List of Instrument Certificates for Environmental Quality Analysis

No.	Instrument/Equipment	Parameter	Manufacturer	Model/Serial No.	Calibrator	Certification No.	Date of Calibration	Due date of Calibration*
1	Atomic Absorption Spectrometer	CADMIUM CHROMIUM CHROMIUM TRIVALENT COPPER LEAD MANGANESE MERCURY NICKEL ZINC	Agilent Technologies	AA240FS / MY13160001	Agilent Technologies (Thailand) Co.,Ltd.	Preventive Maintenance Checklist	30/1/2025	29/1/2026
2	Atomic Absorption Spectrometer	ARSENIC SELENIUM	Perkin Elmer	PinAAcle 900F / PFB20031902	Perkin Elmer Co.,Ltd.	Preventive Maintenance Report	29/4/2025	28/4/2026
3	Analytical Balance	FAT OIL AND GREASE	Mettler Toledo	AB204-S/FACT / 1129361010	United Analyst and Engineering Consultant Co., Ltd.	250422 1 BL002 25	23/4/2025	22/4/2026
4	Analytical Balance	TOTAL DISSOLVED SOLIDS	Mettler Toledo	XSR205DU / C210685394	National Food Institute,Ministry of Industry, Thailand	2502226-002-01	20/3/2025	19/3/2026
5	Analytical Balance	TOTAL SUSPENDED SOLIDS	Mettler Toledo	XSR205DU / C009071872	National Food Institute,Ministry of Industry, Thailand	2502226-001-01	20/3/2025	19/3/2026
6	Auto Clave	TOTAL COLIFORM BACTERIA	ALP Co.,Ltd. (Japan)	CL-40L / 810010	National Food Institute Ministry of Industry (Thailand)	2503287-001-01	5/6/2025	4/6/2026
7	BOD Incubator	BIOCHEMICAL OXYGEN DEMAND	ARCO	UC4-1320 / 13URC4S013201	Technology Promotion Association (Thailand-Japan)	25TM205	8/2/2025	7/2/2026
8	BOD Incubator	BIOCHEMICAL OXYGEN DEMAND	ARCO	UR-1320 / -	Technology Promotion Association (Thailand-Japan)	25TM578	19/3/2025	18/3/2026
9	Continuous Flow Analyzer(CFA)	CYANIDE	Skalar Analytical B.V., the Netherlands	San++5000-02 / 182688	DKSH (Thailand) Ltd.	WO-00074079	23/5/2025	22/5/2026
10	DO Meter	BIOCHEMICAL OXYGEN DEMAND	YSI	5100 / 11B 101863	Technology Promotion Association (Thailand-Japan)	25TW29	17/2/2025	16/2/2026

List of Instrument Certificates for Environmental Quality Analysis

No.	Instrument/Equipment	Parameter	Manufacturer	Model/Serial No.	Calibrator	Certification No.	Date of Calibration	Due date of Calibration*
11	Digestion Units	TOTAL KJELDAHL NITROGEN	Foss Tecator	2520 Auto / 91794469	National Food Institute Ministry of Industry, Thailand	2501440-001-01	27/1/2025	26/1/2026
12	Gas Chromatography	a-BHC ALDRIN b-BHC d-BHC DIELDRIN ENDOSULFAN I ENDOSULFAN II ENDOSULFAN SULFATE ENDRIN ENDRIN ALDEHYDE g-BHC HEPTACHLOR HEPTACHLOR EPOXIDE METHOXYCHLOR pp-DDD pp-DDE pp-DDT	Agilent Technologies	8890 / US2229A024	Agilent Technologies (Thailand) Co.,Ltd.	Preventive Maintenance Checklist	16/6/2025	15/6/2026
13	Mercury Analyzer	MERCURY	NIC. Japan	RA-4500 / 17780278	Coax Group Corporation Ltd.	Preventive Maintenance Report	3/7/2025	2/7/2026
14	Hot Air Oven	TOTAL DISSOLVED SOLIDS TOTAL SUSPENDED SOLIDS	Memmert	UF55 / B212.0411	Technology Promotion Association (Thailand-Japan)	25TM579	19/3/2025	18/3/2026
15	Incubator	TOTAL COLIFORM BACTERIA	Binder	KB400 / 20220000022479	National food institute ministry of Industry	2503682 004 01	1/7/2025	30/6/2026
16	Inductively Coupled Plasma- Optical Emission Spectrometer(ICP-OES)	BARIUM	Agilent Technologies, USA	5110 VDV(G8015AA) / MY18030001	Agilent Technologies (Thailand) Co.,Ltd.	Preventive Maintenance Checklist	4/11/2024	3/11/2025
17	Kjeltec System Distilling Unit	TOTAL KJELDAHL NITROGEN	Foss Tecator (Labtec)	KT200 / 91790524	FOSS South East Asia	13319	27/1/2025	26/1/2026

List of Instrument Certificates for Environmental Quality Analysis

No.	Instrument/Equipment	Parameter	Manufacturer	Model/Serial No.	Calibrator	Certification No.	Date of Calibration	Due date of Calibration*
18	pH Meter	pH	Horiba	LAQUA-PH210 / HA0A0007	technology promotion association (thailand-japan	25CH353	20/3/2025	18/3/2026
19	pH Meter	pH	Horiba	LAQUA-PH210 / HA0A0005	technology promotion association (thailand-japan	24CH1597	26/12/2024	24/12/2025
20	pH Meter	pH	Horiba	LAQUA-PH210 / HA9M0047	technology promotion association (thailand-japan	25CH354	20/3/2025	18/3/2026
21	pH Meter	pH	Horiba	LAQUA-PH210 / HA0D0081	technology promotion association (thailand-japan	25CH736	23/6/2025	22/6/2026
22	Spectrophotometer	CHROMIUM HEXAVALENT COLOUR (pH 7.0) COLOUR (pH Sample)	Agilent	Cary 60 G6860A / MY15410009	DQE Services Co.,Ltd.	SP25-019	26/5/2025	25/5/2026
23	UV-VIS Spectrophotometer	NITRATE NITROGEN PHOSPHATE	Hitachi	U-2900 / 21E22-009	DQE Services Co.,Ltd.	SP25-001	3/1/2025	2/1/2026
24	UV/VIS Spectrophotometer	AMMONIA-NITROGEN CHEMICAL OXYGEN DEMAND FORMALDEHYDE PHENOLS	Hitachi	U-5100 / 23A4-008	DQE Services Co.,Ltd.	SP25-024	17/6/2025	16/6/2026

Due Date of Calibration* : Based on the annual calibration plan. At least 1 time per year.

List of Instrument Certificates for Environmental Quality Analysis

No.	Instrument/Equipment	Parameter	Manufacturer	Model/Serial No.	Calibrator	Certification No.	Date of Calibration	Due date of Calibration*
1	Analytical Balance	PARTICULATE MATTER (PM10) TOTAL SUSPENDED PARTICULATE	Mettler Toledo	MS204TS/00 / C252436235	National Food Institute, Ministry of Industry, Thailand	2502228-003-01	19/3/2025	18/3/2026

Due Date of Calibration* : Based on the annual calibration plan. At least 1 time per year.



Certificate of Calibration

Cert.No.: 24CH1597
Page.: 1 of 3

Equipment : pH Meter
Manufacturer : Horiba
Model : LAQUA-PH210
Serial No. : HA0A0005
ID No. : UAE.EFM.004/2563(EFM.pH.04/63)
Condition As-Received: Used Item
Received Date : 24 December 2024
Calibration Date : 26 December 2024
Reference : 2412.0601WSC-2
Submitted by : United Analyst and Engineering Consultant Co.,Ltd.
3 Soi Udomsuk 41, Sukhumvit Road,
Bangchak, Phrakhanong, Bangkok 10260

Ambient Temperature : (25 ± 2.5) °C
Relative Humidity : (50 ± 15) %
Calibration Procedure : In - house method :
- CP-CH5 by direct measurement with DC voltage
standard and direct measurement with
certified reference material (CRM)
- CP-CH8 by comparison with temperature standard

Calibrated by : Warakorn Lamgagrakul

Approved by :

Approved Signatory

() Pornthippa Tameyakul
() Ponpan Palpim
(✓) Saithip Meangmai

Issue Date : 27 December 2024

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3: Equipment Calibration and Testing Services.

เอกสารไม่ควบคุม



Cert.No.: 24CH1597
Page.: 2 of 3

Condition of this calibration result

Instrument	Serial No.	ID No.	Cert. No.	Due Date
1) Document Process Calibrator	54030049	130RC116	24E2759	25 Aug 2025
2) Ref. Standard Thermometer	4882054	110RC044	24I757	14 July 2025

- This Certification is traceable to SI Through Technology Promotion Association (Thailand - Japan)

2. Certified Reference Materials : The measurement results are traceable to SI through Hach Lenge GmbH Ltd.,
Deutsche Akkreditierungsstelle, Accredited No.D-RM-15184-01-00
: The measurement results are traceable to SI through CPA chem Ltd.,
ANSI-ASQ National Accreditation Board, Accredited No. AR-1835

Buffer Solution	Manufacturer	Lot No.	Exp. date
pH 4.008	CPA chem	1034203	27 Sep 2026
pH 7.000	Hach Lenge GmbH	C03185	09 July 2026
pH 10.010	CPA chem	1034205	27 Sep 2025

3. This certificate is valid only to the item calibrated on date and place of calibration.

Calibration Results

Function : mV Measurement

Performing standard curve by Document Process Calibrator at pH (4,7)(7,10)

Unit Under Calibration	Nominal Value	Standard Voltage Input	Actual Reading		Uncertainty of Measurement (±mV)	Coverage factor k
			pH	mV		
pH Meter S/N.: HA0A0005	4.00	177.48	177.4	4.01	0.058	2.00
	7.00	0.00	0.1	7.00	0.058	2.00
	7.00	0.00	0.1	7.00	0.058	2.00
	10.00	-177.48	-177.2	10.01	0.058	2.00

เอกสารไม่ควบคุม



Cert.No.: 24CH1597
Page.: 3 of 3

Calibration Results

Function : pH Measurement

Performing three buffers standard curve by using buffer nominal pH (4,7)(7,10)

Unit Under Calibration	Standard pH Buffer Solution	Actual pH Reading	Actual mV Reading (mV)	Uncertainty of pH Measurement (±)	Coverage factor k
pH Electrode S/N.: -	4.008	4.01	177.2	0.0079	2.00
	7.000	7.00	2.2	0.0092	2.00
	7.000	7.00	2.2	0.0085	2.00
	10.010	10.01	-170.9	0.0095	2.00

Function : Temperature Measurement

(*) Without adjustment

This equipment was connected with Temperature Probe;

- Model : -

- Serial No. : -

Dimension of probe

- Length : 112 mm.

- Diameter : 16 mm.

- Immersion Depth : 100 mm.

Calibration Point (°C)	Standard Temperature (°C)	UUC* Reading (°C)	Error (°C)	Uncertainty of measurement (± °C)	Coverage factor k
15.0	15.003	15.0	-0.003	0.13	2.00
30.0	30.001	30.0	-0.001	0.13	2.00
45.0	45.002	45.0	-0.002	0.13	2.00

Remark : UUC* = Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k, providing a level of confidence of approximately 95 %.

-000-

เอกสารไม่ควบคุม



Certificate of Calibration

Cert.No.: 25CH353
Page.: 1 of 3

Equipment : pH Meter
Manufacturer : Horiba
Model : LAQUA-PH210
Serial No. : HA0A0007
ID No. : UAE.EFM.002/2563(EFM.pH.02/63)
Condition As-Received: Used Item
Received Date : 18 March 2025
Calibration Date : 20 March 2025
Reference : 2503-0612WSC-1
Submitted by : United Analyst and Engineering Consultant Co.,Ltd.
3 Soi Udomsuk 41, Sukhumvit Road, Bangchak,
Phrakhanong, Bangkok 10260

Ambient Temperature : (25 ± 2.5) °C
Relative Humidity : (50 ± 15) %
Calibration Procedure : In - house method :
- CP-CH5 by direct measurement with DC voltage
standard and direct measurement with
certified reference material (CRM)
- CP-CH8 by comparison with temperature standard

Calibrated by : Uthen Kankawi

Approved by :

Approved Signatory

() Chakrit Waewwanjua
() Ponpan Palpim
(✓) Saithip Meangmai

Issue Date : 20 March 2025

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3: Equipment Calibration and Testing Services.

เอกสารไม่ควบคุม



Cert.No.: 25CH353
Page.: 2 of 3

Condition of this calibration result

1. Reference Standard Instrument

Instrument	Serial No.	ID No.	Cert. No.	Due Date
1) Document Process Calibrator	43160066	130RC092	24E1320	22 Apr 2025
2) Ref. Standard Thermometer	4982054	110RC044	24I757	14 July 2025

- This Certification is traceable to SI Through Technology Promotion Association (Thailand - Japan)

2. Certified Reference Materials : The measurement results are traceable to SI through Hach Lenge GmbH Ltd.,
Deutsche Akkreditierungsstelle, Accredited No.D-RM-15184-01-00
: The measurement results are traceable to SI through CPA chem Ltd.,
ANSI-ASQ National Accreditation Board, Accredited No. AR-1835

Buffer Solution	Manufacturer	Lot No.	Exp. date
pH 4.007	CPA chem	1066665	18 Jan 2027
pH 6.999	Hach Lenge GmbH	C03220	29 Oct 2026
pH 10.010	CPA chem	1066669	18 Jan 2026

3. This certificate is valid only to the item calibrated on date and place of calibration.

Calibration Results

Function : mV Measurement

Performing standard curve by Document Process Calibrator at pH (4,7)(7,10)

Unit Under Calibration	Nominal Value	Standard Voltage Input	Actual Reading		Uncertainty of Measurement (\pm mV)	Coverage factor k
	pH	mV	mV	pH		
pH Meter S/N.: HA0A0007	4.00	177.48	177.6	4.01	0.058	2.00
	7.00	0.00	0.3	6.98	0.058	2.00
	7.00	0.00	0.3	6.98	0.058	2.00
	10.00	-177.48	-177.1	10.01	0.058	2.00



Cert.No.: 25CH353
Page.: 3 of 3

Calibration Results

Function : pH Measurement

Performing three buffers standard curve by using buffer nominal pH (4,7)(7,10)

Unit Under Calibration	Standard pH Buffer Solution	Actual pH Reading	Actual mV Reading (mV)	Uncertainty of pH Measurement (\pm)	Coverage factor k
pH Electrode S/N.: 992H0385	4.007	4.00	150.1	0.0085	2.05
	6.999	7.00	-26.1	0.0095	2.00
	6.999	7.00	-26.7	0.011	2.05
	10.010	10.01	-202.4	0.010	2.00

Function : Temperature Measurement

(*) Without adjustment

This equipment was connected with Temperature Probe;

- Model : 9652

- Serial No. : 992H0385

Dimension of probe

- Length : 103 mm.

- Diameter : 16 mm.

- Immersion Depth : 90 mm.

Calibration Point (°C)	Standard Temperature (°C)	UUC* Reading (°C)	Error (°C)	Uncertainty of measurement (\pm °C)	Coverage factor k
15.0	15.006	15.0	-0.006	0.13	2.00
30.0	29.998	30.0	0.002	0.13	2.00
45.0	44.993	45.0	0.007	0.13	2.00

Remark : - UUC* = Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k, providing a level of confidence of approximately 95 %.

-o0o-

เอกสารไม่ควบคุม

เอกสารไม่ควบคุม



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL.0-2717-3000-29 FAX.0-2719-9484



Certificate of Calibration

Cert.No.: 25CH354
Page.: 1 of 3

Equipment : pH Meter
Manufacturer : Horiba
Model : LAQUA-PH210
Serial No. : HA9M0047
ID No. : UAE.EFM.005/2563 (EFM.pH.05/63)
Condition As-Received: Used Item
Received Date : 18 March 2025
Calibration Date : 20 March 2025
Reference : 2503-0612WSC-2
Submitted by : United Analyst and Engineering Consultant Co.,Ltd.
3 Soi Udumsuk 41, Sukhumvit Road, Bangchak,
Phrakhanong, Bangkok 10260
Ambient Temperature : (25 \pm 2.5) °C
Relative Humidity : (50 \pm 15) %
Calibration Procedure : In - house method :
- CP-CH5 by direct measurement with DC voltage standard and direct measurement with certified reference material (CRM)
- CP-CH8 by comparison with temperature standard

Calibrated by : Uthen Kankawi

Approved by : 
Approved Signatory

() Chakrit Waewwanjua
() Ponpan Paipim
(✓) Saithip Meangmai

Issue Date : 20 March 2025

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

เอกสารไม่ควบคุม



Cert.No.: 25CH354
Page.: 2 of 3

Condition of this calibration result

1. Reference Standard Instrument

Instrument	Serial No.	ID No.	Cert. No.	Due Date
1) Document Process Calibrator	43160066	130RC092	24E1320	22 Apr 2025
2) Ref. Standard Thermometer	4982054	110RC044	24I757	14 Jul 2025

- This Certification is traceable to SI Through Technology Promotion Association (Thailand - Japan)

2. Certified Reference Materials : The measurement results are traceable to SI through Hach Lenge GmbH Ltd.,
Deutsche Akkreditierungsstelle, Accredited No.D-RM-15184-01-00
: The measurement results are traceable to SI through CPA chem Ltd.,
ANSI-ASQ National Accreditation Board, Accredited No. AR-1835

Buffer Solution	Manufacturer	Lot No.	Exp. date
pH 4.007	CPA chem	1066665	18 Jan 2027
pH 6.999	Hach Lenge GmbH	C03220	29 Oct 2026
pH 10.010	CPA chem	1066669	18 Jan 2026

3. This certificate is valid only to the item calibrated on date and place of calibration.

Calibration Results

Function : mV Measurement

Performing standard curve by Document Process Calibrator at pH (4,7)(7,10)

Unit Under Calibration	Nominal Value	Standard Voltage Input	Actual Reading		Uncertainty of Measurement (\pm mV)	Coverage factor k
	pH	mV	mV	pH		
pH Meter S/N.: HA9M0047	4.00	177.48	177.7	4.01	0.058	2.00
	7.00	0.00	0.3	7.01	0.058	2.00
	7.00	0.00	0.3	7.01	0.058	2.00
	10.00	-177.48	-176.8	10.01	0.058	2.00

เอกสารไม่ควบคุม



Cert.No.: 25CH354
Page.: 3 of 3

Calibration Results

Function : pH Measurement

Performing three buffers standard curve by using buffer nominal pH (4,7)(7,10)

Unit Under Calibration	Standard pH Buffer Solution	Actual pH Reading	Actual mV Reading (mV)	Uncertainty of pH Measurement (±)	Coverage factor k
pH Electrode S/N.: -	4.007	4.01	168.5	0.011	2.13
	6.999	7.00	-5.9	0.012	2.09
	6.999	7.00	-6.1	0.011	2.07
	10.010	10.02	-176.7	0.010	2.00

Function : Temperature Measurement

(*) Without adjustment

This equipment was connected with Temperature Probe;

- Model : -

- Serial No. : -

Dimension of probe

- Length : 103 mm.

- Diameter : 16 mm.

- Immersion Depth : 90 mm.

Calibration Point (°C)	Standard Temperature (°C)	UUC* Reading (°C)	Error (°C)	Uncertainty of measurement (± °C)	Coverage factor k
15.0	15.005	15.0	-0.005	0.13	2.00
30.0	30.007	30.0	-0.007	0.13	2.00
45.0	44.995	44.9	-0.095	0.13	2.00

Remark - UUC* = Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k , providing a level of confidence of approximately 95 %.

-00-

เอกสารไม่ควบคุม



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL.0-2717-3000-29 FAX.0-2719-9484



Certificate of Calibration

Cert.No.: 25CH736
Page.: 1 of 3

Equipment : pH Meter
Manufacturer : Horiba
Model : LAQUA-PH210
Serial No. : HAOD0081
ID No. : UAE.EFM.074/2564(EFM.pH.07/64)
Condition As-Received: Used Item
Received Date : 18 June 2025
Calibration Date : 23 June 2025
Reference : 2506-0591WSC-3
Submitted by : United Analyst and Engineering Consultant Co.,Ltd.
3 Soi Udomsuk 41, Sukhumvit Road, Bangkok, Phrakhanong, Bangkok 10260
Ambient Temperature : (25 ± 2.5) °C
Relative Humidity : (50 ± 15) %
Calibration Procedure : In - house method :
- CP-CH5 by direct measurement with DC voltage standard and direct measurement with certified reference material (CRM)
- CP-CH8 by comparison with temperature standard

Calibrated by : Walalak Sirthean

Approved by :
Approved Signatory

() Chakrit Waewwanjua
() Ponpan Paipim
(✓) Saithep Meangmai

Issue Date : 24 June 2025

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

เอกสารไม่ควบคุม



Cert.No.: 25CH736
Page.: 2 of 3

Condition of this calibration result

1. Reference Standard Instrument

Instrument	Serial No.	ID No.	Cert. No.	Due Date
1) Document Process Calibrator	54030049	130RC116	24E2759	25 Aug 2025
2) Ref. Standard Thermometer	4982054	110RC044	24I757	14 July 2025

- This measurement result is traceable to SI through Technology Promotion Association (Thailand - Japan)

2. Certified Reference Materials

:The measurement results are traceable to SI through Hach Lenge GmbH Ltd., Deutsche Akkreditierungsstelle, Accredited No.D-RM-15184-01-00

:The measurement results are traceable to SI through CPA chem Ltd., ANSI-ASQ National Accreditation Board, Accredited No. AR-1835

Buffer Solution	Manufacturer	Lot No.	Exp. date
pH 4.007	CPA chem	1066665	18 Jan 2027
pH 7.000	Hach Lenge GmbH	C03232	02 Dec 2026
pH 10.010	CPA chem	1066669	18 Jan 2026

3. This certificate is valid only to the item calibrated on date and place of calibration.

Calibration Results

Function : mV Measurement

Performing standard curve by Document Process Calibrator at pH (4,7)(7,10)

Unit Under Calibration	Nominal Value	Standard Voltage Input	Actual Reading		Uncertainty of Measurement (±mV)	Coverage factor k
			mV	pH		
pH Meter S/N.: HAOD0081	4.00	177.48	177.4	4.01	0.058	2.00
	7.00	0.00	0.0	6.98	0.058	2.00
	7.00	0.00	0.0	6.98	0.058	2.00
	10.00	-177.48	-177.4	10.01	0.058	2.00



Cert.No.: 25CH736
Page.: 3 of 3

Calibration Results

Function : pH Measurement

Performing three buffers standard curve by using buffer nominal pH (4,7)(7,10)

Unit Under Calibration	Standard pH Buffer Solution	Actual pH Reading	Actual mV Reading (mV)	Uncertainty of pH Measurement (±)	Coverage factor k
pH Electrode S/N.: -	4.007	4.01	176.5	0.0079	2.00
	7.000	6.98	0.8	0.0085	2.00
	7.000	7.00	-0.7	0.0095	2.00
	10.010	10.01	-172.7	0.0092	2.00

Function : Temperature Measurement

(*) Without adjustment

This equipment was connected with Temperature Probe;

- Model : -

- Serial No. : -

Dimension of probe

- Length : 103 mm.

- Diameter : 16 mm.

- Immersion Depth : 90 mm.

Calibration Point (°C)	Standard Temperature (°C)	UUC* Reading (°C)	Error (°C)	Uncertainty of measurement (± °C)	Coverage factor k
15.0	15.000	15.0	0.000	0.13	2.00
30.0	30.000	30.0	0.000	0.13	2.00
45.0	45.003	45.0	-0.003	0.13	2.00

Remark - UUC* = Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k , providing a level of confidence of approximately 95 %.

-00-

เอกสารไม่ควบคุม

เอกสารไม่ควบคุม



Certificate of Calibration

Cert. No.: 25TM205
Page : 1 of 3

Equipment : BOD Incubator
Manufacturer : Arco
Model : UC4-1320
Serial No. : 13URC4S013201
ID No. : UAE.WAO.015/2561
Submitted by : United Analyst and Engineering Consultant Co.,Ltd.
3 Soi Udomsuk 41, Sukhumvit Road
Bangchak, Phrakhanong
Bangkok 10260
Location : Lab. Floor 2
Received Order : 08 February 2025
Calibration Date : 08 February 2025
Ambient Temperature : (26 ± 10) °C
Relative Humidity : (50 ± 30) %
AC Line Voltage : (220 ± 22) V

Calibrated by : Krisda Malee

Approved by :

() Chakrit Waewwanjua
() Suwit Imjai
(✓) Kunchit Promprat

Issue Date : 21 February 2025

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3: Equipment Calibration and Testing Services.

เอกสารไม่ควบคุม



Equipment : BOD Incubator
Condition As-Received : Used Item
Reference : 2502-0166OC-1

Cert. No.: 25TM205
Page : 2 of 3

Procedure Used :-

Calibration were conducted using calibration procedure CP-OT02 based on TLAS G-20 according to direct measurement method with Data Acquisition which connected with Resistance Temperature Detector (RTD).
The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

Instrument	Serial No.	Cert. No.	Traceable	Due Date
1) Data Acquisition	MY57013823	24LM71	TPA	12 May 2025

2. This certificate is valid only to the item calibrated on date and place of calibration.
3. This certification is traceable to the International System of Unit.


Remark : TPA : Technology Promotion Association (Thailand - Japan)

Result of Calibration : (*) Without Adjustment

Function of UUC* : Temperature Source

Fresh air setting : Not Available

Environment during calibration		
	Beginning	Finished
Temp. (°C)	26	25
REL.Humid. (%)	49	52
AC Supply (Volt)	221	220



Probe Installation Details :

a = 10 cm
b = 10 cm
c = 10 cm

Dimension of Chamber :

D = 0.62 m
W = 1.2 m
H = 1.2 m
Capacity = 0.89 m³

Position :	Ref. Std. ID No.:
1	21-17RTD-01
2	21-17RTD-02
3	17RTD-03
4	24-17RTD-04
5	17RTD-05
6	17RTD-06
7	17RTD-07
8	23-17RTD-08
9 (ref.)	23-17RTD-09

เอกสารไม่ควบคุม



Equipment : BOD Incubator
Condition As-Received : Used Item
Reference : 2502-0166OC-1
Result of Calibration : (*) Without Adjustment
Function of UUC* : Temperature Source
Fresh air setting : Not Available

Cert. No.: 25TM205
Page : 3 of 3

Calibration Point (°C)	UUC* Setting (°C)	UUC* Reading (°C)	Temperature stability (± °C)	Temperature uniformity (°C)	Overall Variation (°C)	Coverage Factor k
20.0	20.0	19.9	0.36	0.56	0.99	2

Calibration Point (°C)	Measured Temperature (°C)									Uncertainty (± °C)
	1	2	3	4	5	6	7	8	9 (ref.)	
20.0	19.841	19.714	20.110	19.862	19.747	19.710	19.676	19.789	19.695	0.54

Average* : The average of 30 values in each position.

Temperature stability : One-half of the greatest maximum difference of measured temperature at any one sensor.

Temperature uniformity : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.

Overall Variation : The Difference of the maximum and minimum measured temperatures throughout observation.

UUC* : Unit Under Calibration

Note : The reported uncertainty of measurement was included stability and excluded uniformity .

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k, providing a level of confidence of approximately 95 %.

-o0o-

เอกสารไม่ควบคุม



Certificate of Calibration

Cert. No.: 25TM578
Page : 1 of 3

Equipment : BOD Incubator
Manufacturer : ARCO
Model : UR-1320
Serial No. : -
ID No. : UAE.WAO.006/2553
Submitted by : United Analyst and Engineering Consultant Co.,Ltd.
3 Soi Udomsuk 41, Sukhumvit Road,
Bangchak, Phrakhanong,
Bangkok 10260
Location : Lab Floor 2
Received Order : 19 March 2025
Calibration Date : 19 March 2025
Ambient Temperature : (26 ± 10) °C
Relative Humidity : (50 ± 30) %
AC Line Voltage : (220 ± 22) V

Calibrated by : Man Pattanapongpaiboon

Approved by :

() Chakrit Waewwanjua
() Suwit Imjai
(✓) Kunchit Promprat

Issue Date : 27 March 2025

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3: Equipment Calibration and Testing Services.

เอกสารไม่ควบคุม



Equipment : BOD Incubator
Condition As-Received : Used Item
Reference : 2503-0437OC-2

Cert. No.: 25TM578
Page : 2 of 3

Procedure Used :-
Calibration were conducted using calibration procedure CP-OT02 based on TLAS G-20 according to direct measurement method with Data Acquisition which connected with Resistance Temperature Detector (RTD).
The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument-

Instrument	Serial No.	Cert. No.	Traceable	Due Date
1) Data Acquisition	MY44073381	24LM73	TPA	18 May 2025

2. This certificate is valid only to the item calibrated on date and place of calibration.


3. This certification is traceable to the International System of Unit.

Remark : TPA : Technology Promotion Association (Thailand - Japan)

Result of Calibration :- (*) Without Adjustment

Function of UUC* : Temperature Source

Fresh air setting : Close



Environment during calibration		
	Beginning	Finished
Temp. (°C)	28	28
REL.Humid. (%)	56	55
AC Supply (Volt)	224	224

Position :	Ref. Std. ID No.:
1	1RTD-2/1
2	1RTD-2/2
3	22-01RTD-03
4	1RTD-2/4
5	1RTD-2/5
6	1RTD-2/6
7	23-01RTD-07
8	1RTD-2/8
9 (ref.)	23-01RTD-09

Probe Installation Details :

a = 10 cm
b = 10 cm
c = 10 cm

Dimension of Chamber :

D = 0.62 m
W = 1.2 m
H = 1.2 m
Capacity = 0.89 m³



Equipment : BOD Incubator
Condition As-Received : Used Item
Reference : 2503-0437OC-2
Result of Calibration :- (*) Without Adjustment
Function of UUC* : Temperature Source
Fresh air setting : Close

Cert. No.: 25TM578
Page : 3 of 3

Calibration Point (°C)	UUC* Setting (°C)	UUC* Reading (°C)	Temperature stability (± °C)	Temperature uniformity (°C)	Overall Variation (°C)	Coverage Factor k
20.0	20.0	19.9	0.49	0.69	1.1	2

Calibration Point (°C)	Measured Temperature (°C)									Uncertainty (± °C)
	1	2	3	4	5	6	7	8	9 (ref.)	
20.0	20.025	19.753	20.063	19.839	20.103	20.086	20.152	20.211	19.804	0.69

Average* : The average of 30 values in each position.

Temperature stability : One-half of the greatest maximum difference of measured temperature at any one sensor.

Temperature uniformity : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.

Overall Variation : The Difference of the maximum and minimum measured temperatures throughout observation.

UUC* : Unit Under Calibration

Note : The reported uncertainty of measurement was included stability and excluded uniformity .

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k, providing a level of confidence of approximately 95 % .

-000-

เอกสารไม่ควบคุม

เอกสารไม่ควบคุม



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL.0-2717-3000-29 FAX.0-2719-9484



Certificate of Calibration

Cert. No.: 25TM579
Page : 1 of 3

Equipment : Hot Air Oven

Manufacturer : Memmert

Model : UF 55

Serial No. : B212.0411

ID No. : UAE.WAO.005/2556

Submitted by : United Analyst and Engineering Consultant Co.,Ltd.
3 Soi Udomsuk 41, Sukhumvit Road,
Bangchak, Phrakhanong,
Bangkok 10260

Location : Lab Floor 2

Received Order : 19 March 2025

Calibration Date : 19 March 2025

Ambient Temperature : (26 ± 10) °C

Relative Humidity : (50 ± 30) %

AC Line Voltage : (220 ± 22) V

Calibrated by : Mani Pattanapongpaiboon

Approved by :

() Chakrit Waewwanjua
() Suwit Imjai
(✓) Kunchit Promprat

Issue Date : 27 March 2025



Equipment : Hot Air Oven
Condition As-Received : Used Item
Reference : 2503-0437OC-3

Cert. No.: 25TM579
Page : 2 of 3

Procedure Used :-
Calibration were conducted using calibration procedure CP-OT02 based on TLAS G-20 according to direct measurement method with Data Acquisition which connected with Resistance Temperature Detector (RTD) and Thermocouple Type T.

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument-

Instrument	Serial No.	Cert. No.	Traceable	Due Date
1) Data Acquisition	MY44073381	24LM73	TPA	18 May 2025

2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certification is traceable to the International System of Unit.


Remark : TPA : Technology Promotion Association (Thailand - Japan)

Result of Calibration :- (*) Without Adjustment

Function of UUC* : Temperature Source

Fresh air setting : Close

Environment during calibration		
	Beginning	Finished
Temp. (°C)	27	28
REL.Humid. (%)	49	55
AC Supply (Volt)	221	224



Probe Installation Details :

a = 5.0 cm
b = 5.0 cm
c = 5.0 cm

Dimension of Chamber :

D = 0.50 m
W = 0.80 m
H = 0.75 m
Capacity = 0.30 m³

Ref. Std. ID No.: @ Calibration Point		
Position :	(120,180) °C	(104) °C
1	23-01TC-01	1RTD-2/1
2	23-01TC-02	1RTD-2/2
3	23-01TC-03	22-01RTD-03
4	23-01TC-04	1RTD-2/4
5	23-01TC-05	1RTD-2/5
6	23-01TC-06	1RTD-2/6
7	23-01TC-07	23-01RTD-07
8	23-01TC-08	1RTD-2/8
9 (ref.)	23-01TC-09	23-01RTD-09

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

เอกสารไม่ควบคุม

เอกสารไม่ควบคุม



Equipment : Hot Air Oven
Condition As-Received : Used Item
Reference : 2503-0437OC-3
Result of Calibration : (*) Without Adjustment
Function of UUC* : Temperature Source
Fresh air setting : Close

Cert. No.: 25TM579
Page : 3 of 3

Calibration Point (°C)	UUC* Setting (°C)	UUC* Reading (°C)	Temperature stability (± °C)	Temperature uniformity (°C)	Overall Variation (°C)	Coverage Factor k
104.0	104.0	104.0	0.040	0.43	0.78	2
120.0	120.0	120.0	0.64	1.3	1.6	2
180.0	180.0	180.0	0.49	1.5	1.8	2

Calibration Point (°C)	Measured Temperature (°C)									Uncertainty (± °C)
	1	2	3	4	5	6	7	8	9 (ref.)	
104.0	104.335	104.135	104.363	104.317	103.649	103.738	104.179	104.229	104.025	0.42
120.0	119.575	119.366	119.807	119.905	118.994	119.194	119.888	119.994	120.064	1.1
180.0	180.286	179.510	180.401	180.551	179.281	179.463	180.196	180.451	180.374	1.2

Average* : The average of 30 values in each position.

Temperature stability : One-half of the greatest maximum difference of measured temperature at any one sensor.

Temperature uniformity : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.

Overall Variation : The Difference of the maximum and minimum measured temperatures throughout observation.

UUC* : Unit Under Calibration

Note : The reported uncertainty of measurement was included stability and excluded uniformity .

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k, providing a level of confidence of approximately 95 %.

-o0o-

เอกสารไม่ควบคุม



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3 : EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000 FAX. 0-2719-9484

Certificate of Testing

Cert.No.: 25TW29
Page.: 1 of 2

Equipment : DO Meter
Manufacturer : YSI
Model : 5100
Serial No. : 11B 101863
ID No. : UAE.WAO.004/2554
Received Date : 14 February 2025
Test Date : 17 February 2025
Reference : 2502-0473DSC-1
Submitted by : United Analyst and Engineering Consultant Co.,Ltd.
3 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Laboratory Condition : Temperature (25 ± 5) °C
Humidity (50 ± 20) %
Test Procedure : In - house method : CP-CH9
by Comparison Technique with Azide Modification Method
Tested by : Walalak Sirthean
Approved by :
Approved Signatory
() Chakrit Waewwanjua
() Ponpan Palpim
(✓) Saithip Meangmai
Issue Date : 18 February 2025

เอกสารไม่ควบคุม



Cert.No.: 25TW29
Page.: 2 of 2

Condition of this result of calibration

1. Reference Standard Instruments :

This certification is traceable to the International System of Unit through the reference standards laboratory of Industrial Calibration Center, Technology Promotion Association (Thailand-Japan).

Instruments	Serial No.	ID No.	Certificate No.	Due Date
1. Burette	-	130BU10	23CG1172	22 Mar 2025
2. Balance	14233821	110RC001	24MM131	04 July 2025

2. Standard Material :-

Material	Manufacturer	Lot.No.	Assay
Sodium Thiosulfate 5-Hydrate AR	KEMAUS	2203162447	99.6%

Result : Dissolved Oxygen Meter Adjustment With Air 100 %
Dissolved Oxygen Probe No.: 24F100202

Titration Method (Azide Modification Method) (mg/L)	DO Meter Reading (mg/L)	Standard Deviation (mg/L)
8.22	8.22	0.0055

This report was certified only for the instrument we tested.It is allowable to use for study
Intend to use for advertising and referral purpose is prohibited.This report may not be reproduced
other in full, without written approval of the laboratory

-o0o-

เอกสารไม่ควบคุม

Non-conformity Report, 1481.48, 1481.49, 1481.50, 1481.51, 1481.52, 1481.53, 1481.54, 1481.55, 1481.56, 1481.57, 1481.58, 1481.59, 1481.60, 1481.61, 1481.62, 1481.63, 1481.64, 1481.65, 1481.66, 1481.67, 1481.68, 1481.69, 1481.70, 1481.71, 1481.72, 1481.73, 1481.74, 1481.75, 1481.76, 1481.77, 1481.78, 1481.79, 1481.80, 1481.81, 1481.82, 1481.83, 1481.84, 1481.85, 1481.86, 1481.87, 1481.88, 1481.89, 1481.90, 1481.91, 1481.92, 1481.93, 1481.94, 1481.95, 1481.96, 1481.97, 1481.98, 1481.99, 1482.00, 1482.01, 1482.02, 1482.03, 1482.04, 1482.05, 1482.06, 1482.07, 1482.08, 1482.09, 1482.10, 1482.11, 1482.12, 1482.13, 1482.14, 1482.15, 1482.16, 1482.17, 1482.18, 1482.19, 1482.20, 1482.21, 1482.22, 1482.23, 1482.24, 1482.25, 1482.26, 1482.27, 1482.28, 1482.29, 1482.30, 1482.31, 1482.32, 1482.33, 1482.34, 1482.35, 1482.36, 1482.37, 1482.38, 1482.39, 1482.40, 1482.41, 1482.42, 1482.43, 1482.44, 1482.45, 1482.46, 1482.47, 1482.48, 1482.49, 1482.50, 1482.51, 1482.52, 1482.53, 1482.54, 1482.55, 1482.56, 1482.57, 1482.58, 1482.59, 1482.60, 1482.61, 1482.62, 1482.63, 1482.64, 1482.65, 1482.66, 1482.67, 1482.68, 1482.69, 1482.70, 1482.71, 1482.72, 1482.73, 1482.74, 1482.75, 1482.76, 1482.77, 1482.78, 1482.79, 1482.80, 1482.81, 1482.82, 1482.83, 1482.84, 1482.85, 1482.86, 1482.87, 1482.88, 1482.89, 1482.90, 1482.91, 1482.92, 1482.93, 1482.94, 1482.95, 1482.96, 1482.97, 1482.98, 1482.99, 1483.00, 1483.01, 1483.02, 1483.03, 1483.04, 1483.05, 1483.06, 1483.07, 1483.08, 1483.09, 1483.10, 1483.11, 1483.12, 1483.13, 1483.14, 1483.15, 1483.16, 1483.17, 1483.18, 1483.19, 1483.20, 1483.21, 1483.22, 1483.23, 1483.24, 1483.25, 1483.26, 1483.27, 1483.28, 1483.29, 1483.30, 1483.31, 1483.32, 1483.33, 1483.34, 1483.35, 1483.36, 1483.37, 1483.38, 1483.39, 1483.40, 1483.41, 1483.42, 1483.43, 1483.44, 1483.45, 1483.46, 1483.47, 1483.48, 1483.49, 1483.50, 1483.51, 1483.52, 1483.53, 1483.54, 1483.55, 1483.56, 1483.57, 1483.58, 1483.59, 1483.60, 1483.61, 1483.62, 1483.63, 1483.64, 1483.65, 1483.66, 1483.67, 1483.68, 1483.69, 1483.70, 1483.71, 1483.72, 1483.73, 1483.74, 1483.75, 1483.76, 1483.77, 1483.78, 1483.79, 1483.80, 1483.81, 1483.82, 1483.83, 1483.84, 1483.85, 1483.86, 1483.87, 1483.88, 1483.89, 1483.90, 1483.91, 1483.92, 1483.93, 1483.94, 1483.95, 1483.96, 1483.97, 1483.98, 1483.99, 1484.00, 1484.01, 1484.02, 1484.03, 1484.04, 1484.05, 1484.06, 1484.07, 1484.08, 1484.09, 1484.10, 1484.11, 1484.12, 1484.13, 1484.14, 1484.15, 1484.16, 1484.17, 1484.18, 1484.19, 1484.20, 1484.21, 1484.22, 1484.23, 1484.24, 1484.25, 1484.26, 1484.27, 1484.28, 1484.29, 1484.30, 1484.31, 1484.32, 1484.33, 1484.34, 1484.35, 1484.36, 1484.37, 1484.38, 1484.39, 1484.40, 1484.41, 1484.42, 1484.43, 1484.44, 1484.45, 1484.46, 1484.47, 1484.48, 1484.49, 1484.50, 1484.51, 1484.52, 1484.53, 1484.54, 1484.55, 1484.56, 1484.57, 1484.58, 1484.59, 1484.60, 1484.61, 1484.62, 1484.63, 1484.64, 1484.65, 1484.66, 1484.67, 1484.68, 1484.69, 1484.70, 1484.71, 1484.72, 1484.73, 1484.74, 1484.75, 1484.76, 1484.77, 1484.78, 1484.79, 1484.80, 1484.81, 1484.82, 1484.83, 1484.84, 1484.85, 1484.86, 1484.87, 1484.88, 1484.89, 1484.90, 1484.91, 1484.92, 1484.93, 1484.94, 1484.95, 1484.96, 1484.97, 1484.98, 1484.99, 1485.00, 1485.01, 1485.02, 1485.03, 1485.04, 1485.05, 1485.06, 1485.07, 1485.08, 1485.09, 1485.10, 1485.11, 1485.12, 1485.13, 1485.14, 1485.15, 1485.16, 1485.17, 1485.18, 1485.19, 1485.20, 1485.21, 1485.22, 1485.23, 1485.24, 1485.25, 1485.26, 1485.27, 1485.28, 1485.29, 1485.30, 1485.31, 1485.32, 1485.33, 1485.34, 1485.35, 1485.36, 1485.37, 1485.38, 1485.39, 1485.40, 1485.41, 1485.42, 1485.43, 1485.44, 1485.45, 1485.46, 1485.47, 1485.48, 1485.49, 1485.50, 1485.51, 1485.52, 1485.53, 1485.54, 1485.55, 1485.56, 1485.57, 1485.58, 1485.59, 1485.60, 1485.61, 1485.62, 1485.63, 1485.64, 1485.65, 1485.66, 1485.67, 1485.68, 1485.69, 1485.70, 1485.71, 1485.72, 1485.73, 1485.74, 1485.75, 1485.76, 1485.77, 1485.78, 1485.79, 1485.80, 1485.81, 1485.82, 1485.83, 1485.84, 1485.85, 1485.86, 1485.87, 1485.88, 1485.89, 1485.90, 1485.91, 1485.92, 1485.93, 1485.94, 1485.95, 1485.96, 1485.97, 1485.98, 1485.99, 1486.00, 1486.01, 1486.02, 1486.03, 1486.04, 1486.05, 1486.06, 1486.07, 1486.08, 1486.09, 1486.10, 1486.11, 1486.12, 1486.13, 1486.14, 1486.15, 1486.16, 1486.17, 1486.18, 1486.19, 1486.20, 1486.21, 1486.22, 1486.23, 1486.24, 1486.25, 1486.26, 1486.27, 1486.28, 1486.29, 1486.30, 1486.31, 1486.32, 1486.33, 1486.34, 1486.35, 1486.36, 1486.37, 1486.38, 1486.39, 1486.40, 1486.41, 1486.42, 1486.43, 1486.44, 1486.45, 1486.46, 1486.47, 1486.48, 1486.49, 1486.50, 1486.51, 1486.52, 1486.53, 1486.54, 1486.55, 1486.56, 1486.57, 1486.58, 1486.59, 1486.60, 1486.61, 1486.62, 1486.63, 1486.64, 1486.65, 1486.66, 1486.67, 1486.68, 1486.69, 1486.70, 1486.71, 1486.72, 1486.73, 1486.74, 1486.75, 1486.76, 1486.77, 1486.78, 1486.79, 1486.80, 1486.81, 1486.82, 1486.83, 1486.84, 1486.85, 1486.86, 1486.87, 1486.88, 1486.89, 1486.90, 1486.91, 1486.92, 1486.93, 1486.94, 1486.95, 1486.96, 1486.97, 1486.98, 1486.99, 1487.00, 1487.01, 1487.02, 1487.03, 1487.04, 1487.05, 1487.06, 1487.07, 1487.08, 1487.09, 1487.10, 1487.11, 1487.12, 1487.13, 1487.14, 1487.15, 1487.16, 1487.17, 1487.18, 1487.19, 1487.20, 1487.21, 1487.22, 1487.23, 1487.24, 1487.25, 1487.26, 1487.27, 1487.28, 1487.29, 1487.30, 1487.31, 1487.32, 1487.33, 1487.34, 1487.35, 1487.36, 1487.37, 1487.38, 1487.39, 1487.40, 1487.41, 1487.42, 1487.43, 1487.44, 1487.45, 1487.46, 1487.47, 1487.48, 1487.49, 1487.50, 1487.51, 1487.52, 1487.53, 1487.54, 1487.55, 1487.56, 1487.57, 1487.58, 1487.59, 1487.60, 1487.61, 1487.62, 1487.63, 1487.64, 1487.65, 1487.66, 1487.67, 1487.68, 1487.69, 1487.70, 1487.71, 1487.72, 1487.73, 1487.74, 1487.75, 1487.76, 1487.77, 1487.78, 1487.79, 1487.80, 1487.81, 1487.82, 1487.83, 1487.84, 1487.85, 1487.86, 1487.87, 1487.88, 1487.89, 1487.90, 1487.91, 1487.92, 1487.93, 1487.94, 1487.95, 1487.96, 1487.97, 1487.98, 1487.99, 1488.00, 1488.01, 1488.02, 1488.03, 1488.04, 1488.05, 1488.06, 1488.07, 1488.08, 1488.09, 1488.10, 1488.11, 1488.12, 1488.13, 1488.14, 1488.15, 1488.16, 1488.17, 1488.18, 1488.19, 1488.20, 1488.21, 1488.22, 1488.23, 1488.24, 1488.25, 1488.26, 1488.27, 1488.28, 1488.29, 1488.30, 1488.31, 1488.32, 1488.33, 1488.34, 1488.35, 1488.36, 1488.37, 1488.38, 1488.39, 1488.40, 1488.41, 1488.42, 1488.43, 1488.44, 1488.45, 1488.46, 1488.47, 1488.48, 1488.49, 1488.50, 1488.51, 1488.52, 1488.53, 1488.54, 1488.55, 1488.56, 1488.57, 1488.58, 1488.59, 1488.60, 1488.61, 1488.62, 1488.63, 1488.64, 1488.65, 1488.66, 1488.67, 1488.68, 1488.69, 1488.70, 1488.71, 1488.72, 1488.73, 1488.74, 1488.75, 1488.76, 1488.77, 1488.78, 1488.79, 1488.80, 1488.81, 1488.82, 1488.83, 1488.84, 1488.85, 1488.86, 1488.87, 1488.88, 1488.89, 1488.90, 1488.91, 1488.92, 1488.93, 1488.94, 1488.95, 1488.96, 1488.97, 1488.98, 1488.99, 1489.00, 1489.01, 1489.02, 1489.03, 1489.04, 1489.05, 1489.06, 1489.07, 1489.08, 1489.09, 1489.10, 1489.11, 1489.12, 1489.13, 1489.14, 1489.15, 1489.16, 1489.17, 1489.18, 1489.19, 1489.20, 1489.21, 1489.22, 1489.23, 1489.24, 1489.25, 1489.26, 1489.27, 1489.28, 1489.29, 1489.30, 1489.31, 1489.32, 1489.33, 1489.34, 1489.35, 1489.36, 1489.37, 1489.38, 1489.39, 1489.40, 1489.41, 1489.42, 1489.43, 1489.44, 1489.45, 1489.46, 1489.47, 1489.48, 1489.49, 1489.50, 1489.51, 1489.52, 1489.53, 1489.54, 1489.55, 1489.56, 1489.57, 1489.58, 1489.59, 1489.60, 1489.61, 1489.62, 1489.63, 1489.64, 1489.65, 1489.66, 1489.67, 1489.68, 1489.69, 1489.70, 1489.71, 1489.72, 1489.73, 1489.74, 1489.75, 1489.76, 1489.77, 1489.78, 1489.79, 1489.80, 1489.81, 1489.82, 1489.83, 1489.84, 1489.85, 1489.86, 1489.87, 1489.88, 1489.89, 1489.90, 1489.91, 1489.92, 1489.93, 1489.94, 1489.95, 1489.96, 1489.97, 1489.98, 1489.99, 1490.00, 1490.01, 1490.02, 1490.03, 1490.04, 1490.05, 1490.06, 1490.07, 1490.08, 1490.09, 1490.10, 1490.11, 1490.12, 1490.13, 1490.14, 1490.15, 1490.16, 1490.17, 1490.18, 1490.19, 1490.20, 1490.21, 1490.22, 1490.23, 1490.24, 1490.25, 1490.26, 1490.27, 1490.28, 1490.29, 1490.30, 1490.31, 1490.32, 1490.33, 1490.34, 1490.35, 1490.36, 1490.37, 1490.38, 1490.39, 1490.40, 1490.41, 1490.42, 1490.43, 1490.44, 1490.45, 1490.46, 1490.47, 1490.48, 1490.49, 1490.50, 1490.51, 1490.52, 1490.53, 1490.54, 1490.55, 1490.56, 1490.57, 1490.58, 1490.59, 1490.60, 1490.61, 1490.62, 1490.63, 1490.64, 1490.65, 1490.66, 1490.67, 1490.68, 1490.69, 1490.70, 1490.71, 1490.72, 1490.73, 1490.74, 1490.75, 1490.76, 1490.77, 1490.78, 1490.79, 1490.80, 1490.81, 1490.82, 1490.83, 1490.84, 1490.85, 1490.86, 1490.87, 1490.88, 1490.89, 1490.90, 1490.91, 1490.92, 1490.93, 1490.94, 1490.95, 1490.96, 1490.97, 1490.98, 1490.99, 1491.00, 1491.01, 1491.02, 1491.03, 1491.04, 1491.05, 1491.06, 1491.07, 1491.08, 1491.09, 1491.10, 1491.11, 1491.12, 1491.13, 1491.14, 1491.15, 1491.16, 1491.17, 1491.18, 1491.19, 1491.20, 1491.21, 1491.22, 1491.23, 1491.24, 1491.25, 1491.26, 1491.27, 1491.28, 1491.29, 1491.30, 1491.31, 1491.32, 1491.33, 1491.34, 1491.35, 1491.36, 1491.37, 1491.38, 1491.39, 1491.40, 1491.41, 1491.42, 1491.43, 1491.44, 1491.45, 1491.46, 1491.47, 1491.48, 1491.49, 1491.50, 1491.51, 1491.52, 1491.53, 1491.54, 1491.55, 1491.56, 1491.57, 1491.58, 1491.59, 1491.60, 1491.61, 1491.62, 1491.63, 1491.64, 1491.65, 1491.66, 1491.67, 1491.68, 1491.69, 1491.70, 1491.71, 1491.72, 1491.73, 1491.74, 1491.75, 1491.76,

Date: Jun 27, 2025
Job No.: 11675
Instrument: KT200

Start Finish: 04-00 to 10-00
Travel To Customer (Hrs): 1
Labour (Hrs): 10-00 to 13-00 (3)
Travel From Customer (Hrs): -

Application	Special	Standard
Distributor	Courtesy Visit	Installation
Digital Service	PMA Onboarding	Quote
Internal	Warranty	Repair
Investigate	Sales Support	Remote
		Health Check Visit

PMA Type	Smartcare	Smartcare Pro	Foscare
	Smartcare Advance	Foscare Pro	N/A

Details of Work / Test
- PM -
+ Visual Check
- No leak
- hose change on heater & main switch - ok
+ Ultra heater 10 min Switch without Vio - ok
+ Ultra PM kit & 1 set - ok
+ Function Check
- Power on/off - ok
- Alarm - ok
- Screen - ok
- Indicator - ok
Instrument Ready for Use
OK
Not OK*

Part No.	Batch	Description	Qty
100 99965	11.06.2024	PM kit & KT200 heater Analyser (210)	1
1000 9512	29.03.2024	Heating element Steam	1
15690 111	19.10.2022	Ultra PM kit & 2 set	1

Signed FOSS	Signed Customer
Name	Name

Email: Customer Contact: เอกสารไม่ควบคุม

*Remark:



Certificate No.: 250422-1-BL002-25

Code No.: BL002-25

Page: 2 of 3

Equipment: Electronic Balance
Model: AB204-S/FACT
Serial No.: 1129361010
Max. Capacity: 220 g
Calibration Date: April 23, 2025
Condition As-Received: In Condition

Manufacturer: Mettler Toledo
Readability: 0.0001 g
ID No.: UAE.WAS.002/2552

Condition of Equipment:

Condition of This Result of Calibration:

1. Calibration Method: This instrument was calibrated by method UAE/CP.CAL.006 In-House Method based on UKAS Lab 14: 2022

Reference Standard:

Standard	Model	Serial No.	Calibrated By	Certificate No.	Traceability	Due Date
Standard Weight Class E2 (OIML)	1 mg to 1 kg	8749109122	AMARC	25-009359	Mettler-Toledo	21-Jan-27
Standard Weight Class F1 (OIML)	1 mg to 200 g	11119512	AMARC	24-013840	Mettler-Toledo	04-Feb-26

Instrument	Model	Serial No.	Calibrated By	Certificate No.	Traceability	Due Date
Thermo-Hydro-Baro Meter	MHB-3825D	AK46457	SUCCESS	SG-H-00997/67	Success Gateway	21-Nov-25
Thermo-Hydro-Baro Meter	MHB-3825D	AK46457	TPA	25P795	TPA	25-Feb-26

3. This certification is traceable to SI Unit.

4. This certification was certified only for the instrument we calibrated

5. This result of calibration was found accurate as shown on date and place of calibration.

6. Through the reference standard laboratory of AMARC 25-009359 Calibration 0152


Calibration Result:

1. Repeatability of Reading:

Nominal Value (g)	Standard Deviation of Reading (g)
200*	0.00045

2. Eccentric or off-center loading:

A mass of 100 g was placed and moved to various position on pan
The Balance reading obtained is given in the table.



1 (g)	2 (g)	3 (g)	4 (g)	5 (g)	Maximum Difference (g)
100.0000	99.9996	99.9997	100.0003	100.0005	0.0005

เอกสารไม่ควบคุม



Certificate of Calibration

Certificate No.: 250422-1-BL002-25

Code No.: BL002-25

Page: 1 of 3

Customer Name: United Analyst and Engineering Consultant Co., Ltd.
Address: 3 Soi Udomsuk 41, Sukhumvit Rd., Bang Chak, Phrakhanong, Bangkok 10260

Equipment: Electronic Balance

Manufacturer: Mettler Toledo

Model: AB204-S/FACT

Serial No.: 1129361010

Asset No.: UAE.WAS.002/2552

Building: N/A

Floor: 1

Room: 107

Received Date: April 22, 2025

Date of Calibration: April 23, 2025

Calibration Conditions: Temperature 22.8 °C to 23.4 °C
Humidity 54.8 % to 68.9 %
Pressure 756.6 mmHg to 758.2 mmHg

Calibrated by: Sakkarin Srirahang

Approved by: Suwit Chotnok

Signature:

Issued Date: April 25, 2025

Note: 1) The Uncertainties are for a confidence probability of approximately 95%

2) This Certificate is valid only to the item calibrated on date and place of calibration.

3) This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the United Analyst and Engineering Consultant Co., Ltd. (UAE)

เอกสารไม่ควบคุม



Certificate No.: 250422-1-BL002-25

Code No.: BL002-25

Page: 3 of 3

Equipment: Electronic Balance
Model: AB204-S/FACT
Serial No.: 1129361010
Max. Capacity: 220 g
Calibration Date: April 23, 2025

Manufacturer: Mettler Toledo
Readability: 0.0001 g
ID No.: UAE.WAS.002/2552

Calibration Result: (Continued)

Calibration Range: 0 - 200 g

Calibration Adjustment: Internal Calibration

3. Error of indication from nominal or conventional mass value:

Nominal Value (g)	Reference Value (g)	Indication (g)	Correction (g)	Uncertainty (± mg)	Coverage Factor k
Unload	0.0000000	0.0000	0.0000	0.10	2.05
0.01	0.0100025	0.0099	0.0001	0.10	2.05
0.05	0.0500056	0.0500	0.0000	0.10	2.05
0.1	0.1000012	0.0999	0.0001	0.10	2.05
0.5	0.5000133	0.5000	0.0000	0.10	2.05
1	1.0000105	1.0000	0.0000	0.10	2.05
10	10.000010	10.0000	0.0000	0.11	2.04
40	40.000076	40.0000	0.0000	0.14	2.00
50	50.000056	50.0000	0.0001	0.13	2.00
80	80.000107	80.0000	0.0001	0.18	2.00
100	100.000109	99.9999	0.0002	0.17	2.00
120	120.000015	119.9999	0.0003	0.21	2.00
150	150.000165	149.9998	0.0003	0.24	2.00
160	160.000175	159.9997	0.0005	0.26	2.00
200	200.000129	199.9998	0.0004	0.30	2.00

4. Effect of Tare test:

Tare Load (g)	Test Load (g)	Indication (g)	Correction (g)
100	20.000041	19.9999	0.0001
	40.000076	39.9998	0.0002
	60.000066	59.9997	0.0003
	80.000107	79.9999	0.0002
	100.000168	100.0004	-0.0003

Remarks:

The report uncertainty of measurement was based on standard uncertainty multiplied by coverage factor k, providing a level of confidence of approximately 95%.

เอกสารไม่ควบคุม

Calibration Certificate

Certificate No.: 2502226-001-01
Client name: UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.
Address: 3 Soi Udomsuk 41, Sukhumvit Road,
Bangchack, Prakhonong, Bangkok 10260

Page 1 of 4

Equipment: Electronic Balance

Manufacturer: METTLER TOLEDO

Model: XSR205DU

Serial No.: C009071872

ID No.: UAE.WAO.012/2563

Order No.: 2502226

Operation No.: 2502226-001

Date of Receipt: 19 March 2025

Date of Calibration: 20 March 2025

Calibrated by Mr.Yothin Charoensuk
Scientist

Approved by *for N. Nijarabot*
(Mr.Pheraphat Tuanjit)
Manager, Division of Calibration Laboratory
Responsible for the Technical Management Team

Date of Issue: 25 March 2025

The uncertainties are for a confidence probability of approximately 95%

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the National Food Institute.

FCS-009 Revision: 01 Date: 20-04-65

25026 บ้างการพัฒนาศูนย์บริการห้องปฏิบัติการอุตสาหกรรมอาหาร
25026 โซ 35, ถนนสุขุมวิท, แขวงคลองเตย, เขตคลองเตย, กรุงเทพมหานคร 10703, Thailand
Tel : +66(0) 2462 8588 Fax : +66(0) 2462 8545



nfi.com

Calibration Report

Certificate No.: 2502226-001-01
Equipment: Electronic Balance
Manufacturer: METTLER TOLEDO
Model: XSR205DU
Resolution: 0.00001 g / 0.0001 g
Serial No.: C009071872
ID No.: UAE.WAO.012/2563
Capacity: 82 g / 220 g

Date of Calibration: 20 March 2025

Page 3 of 4

Calibration Results: (Continued)

Calibration Range: 0-80 g

Calibration Adjustment: Internal Calibration

3. Departure from Nominal Value: (Range: 0 - 82 g ; Resolution: 0.00001 g)

Nominal Value (g)	Standard Value (g)	Average Reading (g)	Correction (g)	Uncertainty (± g)	Coverage Factor k
unrated	0.000000	0.000009	0.000009	0.0000089	2.00
0.001	0.001003	0.001000	0.000003	0.0000092	2.00
0.005	0.005002	0.005000	0.000002	0.0000094	2.00
0.01	0.010003	0.010000	0.000003	0.0000091	2.00
0.05	0.049996	0.050000	0.000004	0.0000098	2.00
0.1	0.100011	0.100000	0.000011	0.000011	2.00
0.5	0.500016	0.500000	0.000016	0.000014	2.00
1	1.000003	1.000001	-0.000002	0.000016	2.00
2	2.000023	2.000005	-0.000018	0.000017	2.00
5	5.000015	5.000005	-0.000010	0.000021	2.00
10	10.000009	10.000005	-0.000004	0.000026	2.00
20	20.000030	20.00012	0.00009	0.000037	2.00
30	30.000039	30.00012	-0.00008	0.000050	2.00
50	50.000028	50.00014	-0.00011	0.000068	2.00
80	80.000067	80.00020	-0.00013	0.00011	2.00

FCS-012 Revision: 01 Date: 20-04-65

25026 บ้างการพัฒนาศูนย์บริการห้องปฏิบัติการอุตสาหกรรมอาหาร
25026 โซ 35, ถนนสุขุมวิท, แขวงคลองเตย, เขตคลองเตย, กรุงเทพมหานคร 10703, Thailand
Tel : +66(0) 2462 8588 Fax : +66(0) 2462 8545



nfi.com

Calibration Report

Certificate No.: 2502226-001-01
Equipment: Electronic Balance
Manufacturer: METTLER TOLEDO
Model: XSR205DU
Resolution: 0.00001 g / 0.0001 g
Serial No.: C009071872
ID No.: UAE.WAO.012/2563
Capacity: 82 g / 220 g

Date of Calibration: 20 March 2025

Page 2 of 4

Environment Condition: Ambient Temperature: 21.2 ± 0.6 °C Relative Humidity: 48 ± 3.5 %

Place of Calibration: 208 Balance Room, UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.

Condition of Equipment: Good Condition

Condition of This Results of Calibration:

1. Calibration Method: NFI Method W-MA-001 In-House Method based on UKAS Lab 14 : 2019

2. Reference Standards:

Reference Standard	Model	Serial No.	Calibrated By	Certificate No.	Due Date
Standard Weight Class E2	1mg to 200g	B505567572	TCS	M24041005	19 April 2025
Instrument	Model	Serial No.	Calibrated By	Certificate No.	Due Date
Thermo-Hygro Meter	608-H1	NF1.BTH 01723	Quality Reborn	QR25-0542	10 February 2026

3. This certification is traceable to SI UNIT

4. This certificate was certified only for the instrument we calibrated.

5. This result of calibration was found accurate as shown on date and place of calibration only.

Calibration Results:

1. Repeatability of Reading:

Nominal Value (g)	Standard Deviation of Reading (g)
40	0.0000052
80	0.0000042
100	0.0000000
200	0.0000000

2. Off-Center Error:

A mass of 100 g was placed and moved to various position on pan.

The balance reading obtained is given in the table.

1	2	3	4	5	6	(Maximum Difference)
(g)	(g)	(g)	(g)	(g)	(g)	(g)
100.0001	100.0001	100.0001	100.0001	100.0001	100.0002	0.0001

FCS-012 Revision: 01 Date: 20-04-65

25026 บ้างการพัฒนาศูนย์บริการห้องปฏิบัติการอุตสาหกรรมอาหาร
25026 โซ 35, ถนนสุขุมวิท, แขวงคลองเตย, เขตคลองเตย, กรุงเทพมหานคร 10703, Thailand
Tel : +66(0) 2462 8588 Fax : +66(0) 2462 8545



nfi.com

Calibration Report

Certificate No.: 2502226-001-01
Equipment: Electronic Balance
Manufacturer: METTLER TOLEDO
Model: XSR205DU
Resolution: 0.00001 g / 0.0001 g
Serial No.: C009071872
ID No.: UAE.WAO.012/2563
Capacity: 82 g / 220 g

Date of Calibration: 20 March 2025

Page 4 of 4

Calibration Results: (Continued)

Calibration Range: >80-200 g

Calibration Adjustment: Internal Calibration

3. Departure from Nominal Value: (Range: >80 - 200 g ; Resolution: 0.0001 g)

Nominal Value (g)	Standard Value (g)	Average Reading (g)	Correction (g)	Uncertainty (± g)	Coverage Factor k
90	90.00010	90.00002	-0.00008	0.000015	2.00
100	100.00006	100.00001	0.00005	0.000016	2.00
110	110.00007	110.00001	0.00006	0.000017	2.00
120	120.00009	120.00002	-0.00007	0.000018	2.00
130	130.00010	130.00002	-0.00008	0.000019	2.00
140	140.00013	140.00002	-0.00011	0.000019	2.00
150	150.00009	150.00002	-0.00007	0.000021	2.00
160	160.00010	160.00002	-0.00008	0.000022	2.00
170	170.00012	170.00002	-0.00010	0.000023	2.00
200	200.00013	200.00002	-0.00011	0.000028	2.00

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k, providing a level of confidence of approximately 95 %.

----- End -----

FCS-012 Revision: 01 Date: 20-04-65

25026 บ้างการพัฒนาศูนย์บริการห้องปฏิบัติการอุตสาหกรรมอาหาร
25026 โซ 35, ถนนสุขุมวิท, แขวงคลองเตย, เขตคลองเตย, กรุงเทพมหานคร 10703, Thailand
Tel : +66(0) 2462 8588 Fax : +66(0) 2462 8545



nfi.com

Calibration Certificate

Certificate No.: 2503287-001-01
Client name: UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.
Address: 3 Soi Udomsuk 41, Sukhumvit Road,
Bangchack, Prakanong, Bangkok 10260

Page 1 of 3

Equipment: Autoclave
Manufacturer: ALP
Model: CL-40L
Serial No.: 810010
ID No.: UAE.MIC.032/2565
Order No.: 2503287
Operation No.: 2503287-001
Date of Receipt: 5 June 2025
Date of Calibration: 5 June 2025

Calibrated by Mr.Pheraphat Tuanjit
Scientist
Approved by *P. Jaengharit*
(Miss Freeyaporn Jaengkarnkit)
Vice President, Department of Laboratory Services
Responsible for the Technical Management Team
Date of Issue: 11 June 2025

The uncertainties are for a confidence probability of approximately 95 %.
This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the National Food Institute.

F-CS-009 Revision: 01 Date: 20-04-65

Calibration Report

Certificate No.: 2503287-001-01
Equipment: Autoclave
Model: CL-40L **Serial No.:** 810010
Resolution: 1 °C **ID No.:** UAE.MIC.032/2565
Manufacturer: ALP
Date of Calibration: 5 June 2025

Page 2 of 3

Location: Room 301 Media Preparation, UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.
Environment Condition: Ambient Temperature (26 ± 1) °C
Relative Humidity (55 ± 5) %
Line Voltage (230 ± 5) Volt

Condition of this results of Calibration:

- This instrument was calibrated by insert 3 standard Data loggers with RTD into its autoclave and calibration according to W-TE-018 based on BS 2646-1:2021, Autoclaves for sterilization in laboratories
Part 1: Design, construction, safety and performance - Specification.
- The temperature scale used was based on ITS - 90.
- All data show below were final values and the initial data may be obtained upon request.
- Reference Standard Instrument :

Instrument	Model	Serial No.	Certificate No.	Due Date	Through
Digital Thermometer with RTD (Data Logger)	HiTemp140-PT	T20627	NC-25-03-18-381	11-Mar-26	MADGETECH, INC.
	OM-CP-HITEMP-140	R56916	2502081-002-01	11-Mar-26	NATIONAL FOOD INSTITUTE
	PRTemp140	R38546	2501835-001-01	22-Feb-26	NATIONAL FOOD INSTITUTE

- This certificate is traceable to International System of Units (SI Units).
- This certificate was certified only for the instrument we calibrated.
- This result of calibration was found accurate as shown on date and place of calibration only.
- This standard does not apply to sterilizers or disinfectors used for medical, dental, pharmaceutical.
- Condition of Calibrated item : Good
UUC Description : Setting program function sterilization : STERILIZE/NORMAL
Time of sterilization 20 Minute At 115 and 121 °C
- Result of Calibration : ☒ Without adjustment
☐ After adjustment

F-CS-012 Revision: 01 Date: 20-04-65

Calibration Report

Certificate No.: 2503287-001-01
Equipment: Autoclave
Model: CL-40L **Serial No.:** 810010
Resolution: 1 °C **ID No.:** UAE.MIC.032/2565
Manufacturer: ALP
Date of Calibration: 5 June 2025

Page 3 of 3

Calibration point: 115 and 121 °C

Calibration Condition	Temperature (°C)	Relative Humidity (%)	Line Voltage (Volt)
Min	25.8	50	225
Max	26.8	59	235




Table 1 : Reporting of Temperature

Calibration Point (°C)	Measured Temperature (°C) @ Sensor No. (Sensor No.2 is REF)			Uncertainty ± (°C)
	Std. # 1	Std. # 2 (Ref)	Std. # 3	
115	115.46	115.43	115.42	0.70
121	121.59	121.54	121.51	0.70

Table 2 : Reporting of Characterization Result

UUC* Setting (°C)	UUC* Reading				Stability ± (°C)	Uniformity (°C)	Overall Variation (°C)
	Min (°C)	Max (°C)	Average (°C)	MPA			
115	115	115	115	0.08	0.24	0.17	0.50
121	121	121	121	0.12	0.24	0.19	0.52

Note

The quoted uncertainty include " Stability " and " Loading effect (20% of Uniformity)"
UUC* = Unit Under Calibration
Stability = One-half of the greatest maximum difference of measured temperatures at any one sensors, for at least half an hour after reaching steady state.
Uniformity = The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time.
Overall Variation = The difference of the maximum and minimum measured temperatures throughout observation time.
The report uncertainty of measurement was based on standard uncertainty multiplied by coverage factor k= 2, providing a level of confidence of approximately 95 %.

----- End -----

F-CS-012 Revision: 01 Date: 20-04-65

Calibration Certificate

Certificate No.: 2503682-004-01
Client name: UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.
Address: 3 Soi Udomsuk 41, Sukhumvit Road,
Bangchack, Prakanong, Bangkok 10260

Page 1 of 3

Equipment: CHAMBER (Incubator)
Manufacturer: BINDER
Model: KB 400
Serial No.: 20220000022479
ID No.: UAE.MIC.028/2566
Order No.: 2503682
Operation No.: 2503682-004
Date of Receipt: 1 July 2025
Date of Calibration: 1 July 2025

Calibrated by Mr.Pheraphat Tuanjit
Scientist
Approved by *P. Jaengharit*
(Miss Freeyaporn Jaengkarnkit)
Vice President, Department of Laboratory Services
Responsible for the Technical Management Team
Date of Issue: 3 July 2025

The uncertainties are for a confidence probability of approximately 95 %.
This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the National Food Institute.

F-CS-009 Revision: 01 Date: 20-04-65

Calibration Report

Certificate No.: 2503682-004-01
Equipment: CHAMBER (Incubator)
Model: KB 400 Serial No.: 20220000022479
Resolution: 0.1 °C ID No.: UAE.MIC.028/2566
Manufacturer: BINDER
Date of Calibration: 1 July 2025 Page 2 of 3
Location: Microbiology Laboratory, UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.
Environment Condition:
Ambient Temperature (21 ± 1) °C
Relative Humidity (55 ± 10) %
Line Voltage (230 ± 5) Volt

Condition of this results of Calibration:

- This instrument was calibrated by insert 13 standard thermometer into its chamber and calibration according to W-TE-014 Based on TLAS G-20-1/02-08 (E): Guidelines for Calibration and Checks of Temperature Controlled Enclosures.
- The temperature scale used was based on ITS - 90.
- All data show below were final values and the initial data may be obtained upon request.

Reference Standard Instrument :

Instrument	Model	Serial No./ID No.	Certificate No.	Due Date	Through
Digital Thermometer with sensor	34972A	MY59003377	2501168-001-01	13 January 2026	NATIONAL FOOD INSTITUTE
	RTD	CHP101-203 / RTD#101-203			

- This certificate is traceable to International System of Units (SI Units).
- This certificate was certified only for the instrument we calibrated.
- This result of calibration was found accurate as shown on date and place of calibration only.
- Condition of Calibrated item : Good

UUC Description :

Time of Record : 1 Hour 9 Minute At: 35.0 °C
Fresh air Damper : - Open Position -
X Close Fan 100%
- Not Available

- Result of Calibration : ☒ Without adjustment ☐ After adjustment

P. Jeyapalit
3 July 2025

F-CS-012 Revision: 01 Date: 20-04-63

2008 ปีที่ 35 ถนนสุขุมวิท แขวงคลองเตย เขตคลองเตย กรุงเทพมหานคร 10110
2008 ปีที่ 35 ถนนสุขุมวิท แขวงคลองเตย เขตคลองเตย กรุงเทพมหานคร 10110
Tel : +66(0) 2422 8888 Fax : +66(0) 2422 8844



Calibration Report

Certificate No.: 2503682-004-01
Equipment: CHAMBER (Incubator)
Model: KB 400 Serial No.: 20220000022479
Resolution: 0.1 °C ID No.: UAE.MIC.028/2566
Manufacturer: BINDER
Date of Calibration: 1 July 2025 Page 3 of 3
Calibration point: 35.0 °C
Calibration result:

Table 1 : Reporting of Temperature

Calibration Condition	Temperature (°C)	Relative Humidity (%)	Line Voltage (Volt)
MIN	20.1	45	225.0
MAX	22.0	65	235.0



Table 2 : Reporting of Characterization Result

UUC* Setting (°C)	UUC* Reading (°C)	Temperature Stability ± (°C)	Temperature Uniformity (°C)	Overall Variation (°C)
34.8	34.8	34.8	34.8	0.040
	MIN	MAX	Average	
	34.8	34.8	34.8	0.29

Note: The quoted uncertainty include " Stability " and " Loading effect (20% of Temp Uniformity) "

UUC* = Unit Under Calibration

Stability = One-half of the greatest maximum difference of measured temperatures at any one sensors, for at least half an hour after reaching steady state.

Uniformity = The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time.

Overall Variation = The difference of the maximum and minimum measured temperatures throughout observation time.

The report uncertainty of measurement was based on standard uncertainty multiplied by coverage factor k= 2, providing a level of confidence of approximately 95 %.

----- End -----

P. Jeyapalit
3 July 2025

F-CS-012 Revision: 01 Date: 20-04-63

2008 ปีที่ 35 ถนนสุขุมวิท แขวงคลองเตย เขตคลองเตย กรุงเทพมหานคร 10110
2008 ปีที่ 35 ถนนสุขุมวิท แขวงคลองเตย เขตคลองเตย กรุงเทพมหานคร 10110
Tel : +66(0) 2422 8888 Fax : +66(0) 2422 8844



UAE TOX 009/2566

Agilent CrossLab
From Insight to Outcome

Agilent CrossLab Start Up Services Agilent 8890 Gas Chromatograph Preventive Maintenance Checklist

Agilent Preventive Maintenance provides factory recommended service for your analytical instruments to assure reliable operation and the accuracy of your results.

Initiated by highly trained and certified service engineers using genuine Agilent parts and supplies, Agilent Preventive Maintenance provides everything you need to reduce unplanned downtime and keep your systems operating at their peak. This checklist will be completed at the end of the service and provided to you as a record of the preventive maintenance activities.

Agilent 8890 GC Preventive Maintenance Checklist

Introduction

Customer Information

- Customers should provide all necessary operating supplies upon request or the engineer.
- A customer representative should be available to the engineer while performing the preventive maintenance procedures.
- Any parts, not included in the Parts Lists section of this document, are not part of the recommended Preventive Maintenance service, nor are they included in the price of this service.
- A system requires the use of valid or approved procedures and parts for the maintenance additional costs.

Important Customer Web Links

- For more information about Agilent Technologies services, please visit our website using the following URL: <http://www.agilent.com/en-us/products/crosslab-instrument-services/service-repair>
- The Agilent Community is an excellent place to get answers, collaborate with others about applications and Agilent products, and find in-depth documents and videos relevant to Agilent technologies. Visit <https://community.agilent.com/welcome>.
- To access Agilent University, visit <http://www.agilent.com/crosslab/university/> to learn about training options, which include online, classroom and onsite delivery. A training specialist can work directly with you to help determine your best options.
- A useful Agilent Resource Center web page is available, which includes short videos on maintenance, quick lists of consumables for new instruments, and other valuable information. Check out the Resource Page here: <https://www.agilent.com/en-us/agilentresources>.
- Need technical support, FAQs, supplies? – visit our Support Home page <http://www.agilent.com/search/support>.
- Videos about specific preparation requirements for your instrument can be found by searching the Agilent YouTube channel at <https://www.youtube.com/user/agilent>.

Agilent

Revision: 2.01, Issued: September 14, 2021
Agile Document Number: D0013610
DE number: 44166.759722222
© Agilent Technologies, Inc. 2021

Page 2 of 9 **Agilent**

เอกสารไม่ควบคุม

เอกสารไม่ควบคุม

Service Engineer's Responsibilities

- Contact the customer and ensure that all necessary supplies are available before the preventive maintenance visit.
- Only select those pages that relate to the system or module being serviced.
- Complete empty fields with the relevant information.
- Complete the relevant checkboxes in the checklist using either a "X" or tick mark "✓".
- Check "Section not applicable" check boxes to indicate services/tasks not delivered, as appropriate.
- Complete the Preventive Maintenance service in the order of the tasks listed.
- Complete the Service Review section together with the customer.
- Complete the fields for page numbers at the foot of each selected page.
- Complete the total number of pages field in the Service Completion section.
- Ask the customer to sign the Service Completion section including the customer's and your signature.

Additional Instruction Notes

- Check for any active service notes for this unit. If there are any applicable "Safety" or "Modification Recommended" Service notes, plan to implement the changes on this unit before doing any qualification service.
- Do not implement firmware updates, unless you get approval from the customer and are sure that they are compatible with the instrument control software.

Revision: 2.01, Issued: September 14, 2021
Agile Document Number: D0013610
DE number: 44166.759722222
© Agilent Technologies, Inc. 2021

Page 9 of 9



เอกสารไม่ควบคุม

System Information

- ☒ Check this box if an instrument configuration report is attached instead of completing the table below.

Instrument System Name and ID	UAE-TOX 009/2366 / US2229A024
Instrument System Site and Location	UAE / room 404

List System Component Product Numbers	List the Serial Numbers of each Component
1. B454A	US2229A024
2. G4519A	CN22285350
3. G4514A	CN22287018
4.	
5.	
6.	
7.	
8.	
9.	
10.	

Preparation

- ☒ Discuss any specific issues with the customer before starting.
- ☒ Review the instrument logbook for recorded problems and comments.
- ☒ Save instrument control settings before starting the procedure.
- ☒ Perform a general inspection of the system for cleanliness.
- ☒ Check for proper installation of parts, assemblies, sensors etc.
- ☒ Check system for required installation of components, settings as defined by current Service Notes.
- ☒ Check for required firmware updates and verify with customers if they would like them installed.
- ☒ Before starting the following procedures, record the Detector Signal Output(s) in the results table. If the GC is turned OFF or in a service mode, comparing the detector outputs before and after the service is not possible.

Revision: 2.01, Issued: September 14, 2021
Agile Document Number: D0013610
DE number: 44166.759722222
© Agilent Technologies, Inc. 2021

Page 4 of 9



เอกสารไม่ควบคุม

Preventive Maintenance Procedure

Clean and inspect GC

- ☒ Unplug power cord from the power source.
- ☒ Open GC covers and vacuum/remove any dust/debris. Pay particular attention to cooling fans.
- ☒ Inspect internal connectors for proper contact and placement.
- ☒ Reconnect Power to the GC. Power the GC on and verify the power on self-test passed.
- ☒ Verify oven motor spins freely and turns on with the oven door closed; off when the door is opened.
- ☒ Verify operation of all other fans - the inlet and EPC cooling fans.
- ☒ Verify oven intake/outlet flap assembly is operating smoothly while heating and cooling the oven

Inlet and detector consumable replacement

- ☒ Replace the split vent trap assembly if the inlet and detector maintenance procedures from the Browser User interfaces on units with these Inlet: Split/Spillless Capillary (SSL), Multi-Mode Inlet (MMI), Programmed Temperature Vaporizer (PTV), Volatiles Interface (VI).
- ☒ If the inlet system is used in Split Mode with viscous samples, inspect and clean the split vent tube on the inlet and flush or replace the tubing between the inlet and the split vent trap.
- ☒ For the inlets installed, perform inlet maintenance using the Maintenance procedure from the Browser user interfaces. Record the results. (Leak and Restriction test).
- ☒ If the GC includes a Flame Ionization Detector (FID), replace the jet. If the ignitor shows any buildup of sample or corrosion, replace the ignitor. Examine the FID collector and castle assemblies for contamination - clean as necessary.

Zero Sensors and Leak test

- ☒ Zero all pressure sensors using the Browser interface.
- ☒ Perform inlet pressure decay test(s) from the diagnostics screen on the Browser User interface. Record if test passed or failed in the results table.

Note: If the PM is done in preparation for an Operational Qualification, then the pressure decay test defined within that protocol can be used for the PM.

Revision: 2.01, Issued: September 14, 2021
Agile Document Number: D0013610
DE number: 44166.759722222
© Agilent Technologies, Inc. 2021

Page 5 of 9



เอกสารไม่ควบคุม

ALS Maintenance

- ☐ Section NOT applicable
- ☒ Check all cabling and configuration settings between GC, tray, and injectors.
- ☒ Vacuum or remove any dust, especially around fans.
- ☒ Check operation of all fans.
- ☒ Check syringe for smooth plunger operation.
- ☒ Check for smooth operation of the needle support - clean if necessary

Restore Instrument

- ☒ Restore the normal operating conditions or customer method using the Browser interface or Data System.
- ☒ Purge the system with carrier flow for 15 minutes
- ☒ Bake out the system, then restore the normal operating conditions.
- ☒ After equilibration, check and record the post PM detector signal output values. Result should be similar or lower than the detector outputs recorded prior to PM.
- ☒ Perform a chemical checkout. If this is a routine PM, inject the customer's sample using the ALS if applicable. This will act as a final checkout of both the ALS and the GC.

Note: If the PM Service is performed prior to a qualification service, then use the qualification procedure as a guide for final instrument set up and checkout.

Revision: 2.01, Issued: September 14, 2021
Agile Document Number: D0013610
DE number: 44166.759722222
© Agilent Technologies, Inc. 2021

Page 6 of 9



เอกสารไม่ควบคุม

Signature Page

Service Review

- ☐ Attach available reports/printouts of all tests to this documentation.
- ☒ Record the Preventive Maintenance service activity in the customer's records/logbook.
- ☒ Update/reset instrument maintenance counters as appropriate.
- ☒ Affix the PM sticker to the system or instrument logbook based on the customer's request.
- ☒ Complete the Service Engineer Comments section if there are additional comments.
- ☒ Review with the customer this service, parts replaced, and test results obtained.
- ☒ If the instrument firmware was updated, record the details of the change in the Service Engineer's Comments box or if necessary, in the customer's IQ records.
- ☐ Supply the customer with a copy of the Smart Alerts flyer.
- ☐ Describe Smart Alerts to the customer.
- ☐ Install Smart Alerts if requested.

PM Test Results Table

Test description	Before PM Service	After PM Service
Front detector output	N/A	249.11 Hz
Back detector output	N/A	14.9 Hz
AUX 1 detector output	N/A	N/A
AUX 2 detector output	N/A	N/A
Test description	Expected test result	Actual test result
Leak and Restriction Test after front inlet maintenance	Pass	Pass
Leak and Restriction Test after back inlet maintenance	Pass	Pass
Leak and Restriction Test after front inlet Split Vent Trap replacement	Pass	Pass
Leak and Restriction Test after back inlet Split Vent Trap replacement	Pass	Pass
Front inlet pressure decay test	Pass	Pass
Back inlet pressure decay test	Pass	Pass

Revision: 2.01, Issued: September 14, 2021
 Agile Document Number: D0013610
 DE number: 44166.759722222
 © Agilent Technologies, Inc. 2021

Page 7 of 9



เอกสารไม่ควบคุม

PM Parts List Table

Note: The following kits are recommended for capillary and purged packed inlets. If this is a general PM and the customer has a preferred set of consumables, you may use the customer's consumables.

Part description	Part number	Product or model# where used	Quantity consumed
SSL Capillary Inlet PM kit, Splitless	5188-6497	8890 GC	N/A
SSL Capillary Inlet PM kit, Split	5188-6496	8890 GC	1
SSL Capillary Ultra Inert Inlet Gold Seal with Washer	5190-6144	8890 GC	N/A
SSL Capillary Ultra Inert Inlet Splitless Liner - Single taper with Glass Wool	5190-2293	8890 GC	N/A
SSL Capillary Ultra Inert Inlet Low Pressure Drop Split Liner - with Glass Wool	5190-2295	8890 GC	N/A
PP Inlet PM kit	5188-6498	8890 GC	N/A
Split vent trap PM kit, single cartridge (for MMI, PTV & VI)	5188-6495	8890 GC	N/A
MMI Cleaning Kit	G3510-60820	8890 GC	N/A
PTV Septumless Head Rebuild Kit	5182-9747	8890 GC	N/A
PTV Septumless Head Ignition Guide Ignitor (glow plug) assembly with O-ring	5182-9748	8890 GC	N/A
19231-60680		8890 GC	1
FID Collector Rebuild/Cleaning Kit	G1531-67000	8890 GC	N/A
FID Collector Replacement Kit	G1531-67001	8890 GC	N/A
Standard .011-inch FID Jet	5200-0176	8890 GC	1
Universal .018-inch FID Jet	5200-0177	8890 GC	N/A

Revision: 2.01, Issued: September 14, 2021
 Agile Document Number: D0013610
 DE number: 44166.759722222
 © Agilent Technologies, Inc. 2021

Page 8 of 9



เอกสารไม่ควบคุม

Service Engineer Comments

If there are any specific points you wish to note as part of performing the service or other items of interest for the customer, please write include them in this box.

Service Completion

Service request number 60959060 Date service completed 16 June 2025

Agilent signature [Signature] Customer signature [Signature]

Total number of pages in this document 9 pages

Revision: 2.01, Issued: September 14, 2021
 Agile Document Number: D0013610
 DE number: 44166.759722222
 © Agilent Technologies, Inc. 2021

Page 9 of 9



เอกสารไม่ควบคุม

United Analyst and Engineering Consultant Co., Ltd.

Automatic Mercury Analyzer

Model : RA-4500

Preventive Maintenance Report

SERIAL No. RA-4500 : 11780278

Soft version : Ver 2.0.5

ROM version : Ver 2.0.2

DATE : 02 JULY 2025

DUE DATE : 02 JULY 2026

INSPECTED BY : Nattaphong P.
 (Nattaphong P.)

APPROVED BY : [Signature]
 (Kitichai S.)

Kinetic Solutions Company Limited.
 2, Soi Lat Krabang 1, Lat Krabang Subdistrict,
 Lat Krabang District, Bangkok 10520
 Tel. (+66) 062-789-5221



เอกสารไม่ควบคุม

Inspection

ITEMS		SPECIFICATIONS	RESULT	JUDGE
1. Quantity	-	Accessories are completed.	GOOD	OK
2. Appearance	2.1 Overall Appearance	No visible damage.	GOOD	OK
	2.2 Parts / Cables	Correctly placed and connected.	GOOD	
3. Indication	Nameplate / Label	Plate and Label are indicated.	GOOD	OK
4. Self check				
4.1 GLP Counter	Mercury Lamp	5000 hours	110 hr	OK
	Membrane Filter	2000 hours or 1 year after replace	< 1 hr	OK
	Main Pump Tube	750 hours or 1 year after replace	< 1 hr	OK
	Absorbed Hg	1500 mg	< 1 hr	OK
	P1 Tube	2000 hours or 1 year after replace	< 1 hr	OK
	P2 Tube	2000 hours or 1 year after replace	< 1 hr	OK
	P3 Tube	2000 hours or 1 year after replace	< 1 hr	OK
	P4 Tube	2000 hours or 1 year after replace	< 1 hr	OK
	P5 Tube	2000 hours or 1 year after replace	< 1 hr	OK
	P6 Tube	2000 hours or 1 year after replace	< 1 hr	OK
	P7 Tube	2000 hours or 1 year after replace	< 1 hr	OK
	Heater	2000 hours	42 hr	OK
4.2 Check/Test	Flow rate Adjustment	Flow rate 0.14 - 0.20 L/min	0.18 L/min	OK
		V.SIG is 3.5 - 4.5 V.	4.03 V.	OK
	Signals Detector	V.REF is 3.5 - 4.5 V.	4.03 V.	OK
	Cooling Fan	Check the operation of cooling fan	PASS	OK
	Color Sensor	signals (R,G,B) at least one nonzero	PASS	OK
	Radiation Thermometer	a positive valve form thermometer	PASS	OK
Heater	Temperature	At 95°C ± 2°C with 30 min.	94.7°C	OK
6. Calibration Curve	no pretreatment	0-10ng : Max.Dev. 5.0%	0.90%	OK
7. Repeatability	100 µg/L (n=5)	Average: 100 ± 5 µg/L	101.4 µg/L	OK
		C.V. ± 5.0%	0.71%	OK
8. Blank	no pretreatment	Less than 0.5 (AREA)	0.103 AREA	OK

NAME		Date Certified	Expiration
Mercury ICP Standard (1000 µg/mL) AccuStandard, Inc. Lot 223035027		March 10, 2023	March 10, 2028

เอกสารไม่ควบคุม


Inspection details

Remark	
1. Cleaning Mercury Analyzer RA-4500	
- Body case, Cell Detector, Table of Sample	
2. Replace consumable one year set for RA-4500	
3. Checking Mercury Analyzer RA-4500	
- Mercury Lamp	- Outlet Activated Carbon Filter
- Membrane Filter	- Flow Sensor
- Main Pump Tube	- Valves
- Motor Pump	- Heater
- Motor Reagent pump	- Cooling Fan
- Motor of Arm	- Stirrer motor
- Motor of Table	- Color sensor
- Motor of Lift	- Instrument Performance
4. Adjust Optical system	
5. Inspection Calibration curve and Repeatability of Mercury Analyzer RA-4500	
หมายเหตุ Heater Box เริ่มเสื่อมสภาพ แนะนำให้เปลี่ยนในรอบ PM ถัดไป	


เอกสารไม่ควบคุม

Title : Preventive Maintenance
Date : 02/07/2025
Name : Kinetic Solutions
Memo : Calibration curve 0-10ng

Method
Method1 (Pretreatment: without)
(1+1)H2SO4 : 0.9mL
10w/v% SnCl2 : 0.5mL
Measurement Time (sec) : 120sec




No.	STD [µg/L]	SVOL [mL]	CVOL [mL]	DVOL [mL]	STD [ng]	AREA [ON]	MEAS [ng]	Dev [%]	Note
1	0.000	5.000	5.000	5.000	0.000	0.1107	0.0000	-	
2	100.000	0.025	5.000	5.000	2.500	3.2690	2.4250	3.0	
3	100.000	0.050	5.000	5.000	5.000	6.5434	4.9392	1.2	
4	100.000	0.075	5.000	5.000	7.500	9.8649	7.4895	0.1	
5	100.000	0.100	5.000	5.000	10.000	13.2088	10.0570	0.6	

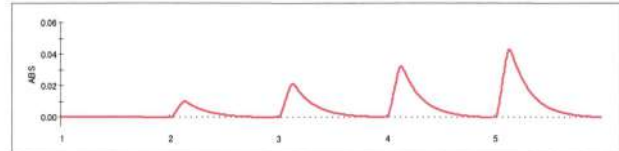

No.	NAME	SVOL [mL]	CVOL [mL]	DVOL [mL]	AREA [ON]	MEAS [ng]	CONC [µg/L]	Note
1	STD 100 ppb	0.050	5.000	5.000	6.7338	5.0854	101.708	
2	STD 100 ppb	0.050	5.000	5.000	6.7129	5.0693	101.386	
3	STD 100 ppb	0.050	5.000	5.000	6.6370	5.0110	100.220	
4	STD 100 ppb	0.050	5.000	5.000	6.7489	5.0970	101.940	
5	STD 100 ppb	0.050	5.000	5.000	6.7514	5.0989	101.978	
6	Blank	5.000	5.000	5.000	0.1035	-0.0055	0.000	

No.	NAME	TRY	AV [µg/L]	SD [µg/L]	Cv [%]
1	STD 100 ppb	5	101.4464	0.724979	0.71


เอกสารไม่ควบคุม

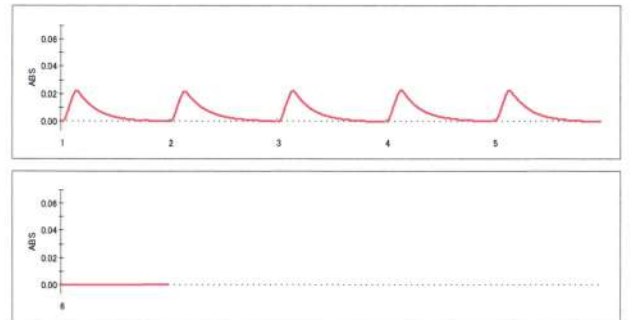

Self Check
Heat check: PASS!! (25.7degC[05:00] -> 29.7degC[02:29])
Sensor check: PASS!! (253- [5= 238])
Leak check: PASS!! (0.18L/min)
Sig/Ref check: PASS!! (Sig: 4.03V, Ref: 4.03V)
Drift check: PASS!! (0.0000637 - -0.0000026 = 0.0000663)

เอกสารไม่ควบคุม

125 Market Street
New Haven, CT 06513
USA

**AccuStandard® Inc.**
Tel: (203) 786-5290
Fax: (203) 786-5339
www.AccuStandard.com


CERTIFICATE OF ANALYSIS

AccuTrace™ Reference Standard

Catalog No: ICP-34N-1
Description: Mercury ICP Standard
Element: Mercury (Hg)
SRM: 3133
Lot: 223035027
Matrix: 10% Nitric acid
Hazards: Refer to SDS for complete safety information

Date Certified: Mar 10, 2023
Expiration: Mar 10, 2028
Density: 1.052 g/mL
Sample Size: 100 mL
Components: 1
Storage Condition: Ambient (>5 °C)


Signal Word: Danger


AP-1463

Certified Concentration: 1000 µg/mL

Trace Elements in µg/mL															
Ag nd<0.02	Ce nd<0.2	Gd nd<0.02	Lu nd<0.02	Pb nd<0.2	Sc nd<0.02	Ti nd<0.02									
Al nd<0.02	Co nd<0.02	Ge nd<0.2	Mg nd<0.02	Pd nd<0.2	Se nd<0.2	Tl nd<0.2									
As nd<0.2	Cr nd<0.02	Hf nd<0.02	Mn nd<0.02	Pr nd<0.2	Si N/A	Tm nd<0.02									
Au nd<0.02	Cs N/A	Hg *	Mo nd<0.02	Pt nd<0.2	Sm nd<0.2	U nd<0.2									
B nd<0.2	Cu nd<0.02	Ho nd<0.02	Na nd<0.02	Rb N/A	Sr nd<0.02	V nd<0.02									
Ba nd<0.02	Dy nd<0.02	In nd<0.2	Nb nd<0.2	Ra nd<0.2	Te nd<0.02	W nd<0.2									
Be nd<0.02	Er nd<0.02	Ir nd<0.2	Nd nd<0.02	Rh nd<0.2	Ta nd<0.2	Y nd<0.02									
Bi nd<0.2	Eu nd<0.02	K nd<0.2	Ni nd<0.02	Ru nd<0.02	Tb nd<0.02	Yb nd<0.02									
Cd nd<0.02	Fe nd<0.02	La nd<0.02	Os N/A	S N/A	Th nd<0.2	Zn nd<0.02									
Ce nd<0.02	Ga nd<0.02	Li nd<0.02	P N/A	Sb nd<0.2	Ti nd<0.02	Zr nd<0.02									

This Certified Reference Material was verified in accordance with ISO/IEC 17025 (AT-1339) and ISO 17034 (AR-1463). This solution was assayed gravimetrically using a balance calibrated against weight sets, ID #86270, traceable to NIST. A product with a suffix (-1A, -2B, etc. or -01, -02, etc.) on its lot number has had its expiration date extended and is identical to the same lot number without the suffix.

This product contains mercury and **MUST** be disposed of in accordance with all federal, state and local regulations.

The gravimetric uncertainty for this product is ±0.24%. The CRM uncertainty is ±2.4%.

In order to verify the concentration(s), the final solution was checked by plasma emission spectroscopy (ICP) against material traceable to the above listed NIST SRM(s).

We use the highest purity raw materials available to minimize impurity levels in the final solution. Typically 99.999%+ pure starting materials are used as well as high purity acids and ASTM Type 1 18 megohm deionized water.


All trace level elemental impurities were determined via plasma emission spectroscopy on the concentrate.

All weights are traceable through NIST. Test No. 684/291344-18 & 684/292805-19

All glassware used in preparation is Class A.

All bottles are acid leached and triple rinsed with deionized water prior to use.

Shake bottle prior to use and do not pipette directly out of the bottle. Use only cleaned Class A volumetric glassware. Keep bottle tightly capped.

Certified By: 
Margaret O'Leary, Inorganic QA Manager

Page 1 of 1

For use in routine laboratory analysis

AccuStandard is accredited to ISO 17034, ISO/IEC 17025 and certified to ISO 9001:2015

เอกสารไม่ควบคุม

- Quality Standards:**
ISO 17034:2016 – General Requirements for the Competence of Reference Material Producers
ISO/IEC 17025:2017 – General Requirements for the Competence of Testing And Calibration Laboratories
ISO 9001:2015 – Quality Management System – Requirements
Eagle Registrations
- Intended Use:** The product covered by this certificate is designed for calibration or for use in quality control procedures for the specified chemical compounds listed on the reverse side. This product can be used for quantification and/or identification. This product can also be used as a reference material to validate analytical procedures, subject to the conditions under Section 7.
- Manufacturing:** All balances are calibrated daily using an in-house procedure with weights that are compared annually to master weights and traceable to NIST. The balances are also calibrated annually by an ISO/IEC 17025 accredited calibration laboratory. Please refer to the NIST test number listed on the front of this certificate. Class A glassware is used in the manufacture and quality control of all standards. Good Laboratory Practices have been used throughout the preparation of this Standard.
- Homogeneity:** This product is sufficiently homogeneous and any sample size would be within the uncertainty budget.
- Stability:** The manufacturer guarantees the stability of this solution through the expiration date stated on the label, when handled and stored according to the conditions stated on the label.
- Uncertainty:** The uncertainty values as stated on the face of this certificate have been determined using the EURACHEM/CITAC Guide. We report a combined expanded uncertainty equal to the positive square root of the total variance of the uncertainty of the components using the following formula: $u_c = \sqrt{(u_1(V))^2 + (u_2(m))^2 + (u_3(V))^2 + (u_4(R))}$. This formula represents uncertainty components from the mass, volume, short-term stability, long-term stability and homogeneity factors associated with the production of this product. The expanded uncertainty, assumes a normal distribution and a coverage factor of $k=2$ is chosen using approximately a 95% confidence level.
- Legal Notice and Limit of Liability:** This product is for routine laboratory analysis and research purposes only. The company's liability will be limited to replacement of product or refund of purchase price. Notice of claims must be made within thirty (30) days from date of delivery.

เอกสารไม่ควบคุม

DQE Services Co., Ltd.

**DQE Services**

32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Bangkok 10230

Phone : +66 (0)2 538 2054, Email : dqeservicesinfo@gmail.com


NIST-17034-17025
CALIBRATION DATA

CERTIFICATE OF CALIBRATION

Certificate No. : SP25-001

Page 1 of 5

Customer : United Analyst and Engineering Consultant Co.,Ltd. (Head Office)

Address : 3 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260

Location of calibration : Laboratory 213

Equipment : UV-Vis Spectrophotometer

Manufacturer : Hitachi

Model : U-2900

Serial No. : 21E22-009


ID No. : UAE.WAT.051/2564

Received Date : 3 January 2025

Calibration Date : 3 January 2025

Issue Date : 8 January 2025

Condition Instrument : Good

Calibrated by : 
(Mr. Tanawut Ritidach)
Technical Manager

Approved by : 
(Ms. Chonthicha Sangerng)
Quality Manager

The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only.

The measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of DQE Services Co., Ltd.

เอกสารไม่ควบคุม

FM-708-02 R01 1/11/2021

DQE Services Co., Ltd.

**DQE Services**

32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Bangkok 10230

Phone : +66 (0)2 538 2054, Email : dqeservicesinfo@gmail.com


NIST-17034-17025
CALIBRATION DATA

REPORT OF CALIBRATION

Certificate No. : SP25-001

Page 2 of 5

Environment Condition : Ambient Temperature 25 ± 5 °C

Relative humidity 55 ± 20 %RH

Calibration method : In-house method CP-01 Based on ASTM E275-08

Certified Reference Materials :

Material	Serial No.	Certificate No.	Due date
Absorbance Standard set	25760	115663	25 October 2025
Absorbance Standard set	25757	115638	25 October 2025
Wavelength Standard set	25806	115657	25 October 2025
Wavelength Standard set	25758	115665	25 October 2025

Traceability : This certification is traceable to the International System of Unit maintained at National -
Institute of Standards and Technology (NIST) through Starna Scientific Limited

Spectral Band Width of UUC : 1.5 nm.

Scan Speed of UUC : 200 nm/min

Scan Interval of UUC : 0.1 nm.



Resolution of UUC : Photometric 0.001 Abs.

Wavelength 0.1 nm.

เอกสารไม่ควบคุม

FM-708-02 R01 1/11/2021

DQE Services Co.,Ltd.
32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Bangkok 10230
Phone : +66 (0)2 538 2054, Email : dqeservicesinfo@gmail.com



REPORT OF CALIBRATION

Certificate No. : SP25-001Page 3 of 5

Calibration Results : Without adjustment



Photometric Accuracy :

Wavelength (nm.)	CRMs Values (Abs)	UUC Reading (Abs)	Correction (Abs)	Uncertainty (Abs)	Coverage factor k
420	0.0000	0.000	0.0000	0.0028	2.00
	0.5780	0.578	0.0000	0.0031	2.00
	1.0484	1.045	0.0034	0.0029	2.00
	2.1876	2.192	-0.0044	0.0075	2.00
440	0.0000	0.000	0.0000	0.0028	2.00
	0.5595	0.560	-0.0005	0.0034	2.00
	1.0239	1.023	0.0009	0.0035	2.00
	2.1230	2.125	-0.0020	0.0079	2.00
465	0.0000	0.000	0.0000	0.0028	2.00
	0.5230	0.521	0.0020	0.0030	2.00
	0.9633	0.961	0.0023	0.0029	2.00
	1.9753	1.977	-0.0017	0.0070	2.00
546.1	0.0000	0.000	0.0000	0.0028	2.00
	0.5181	0.518	0.0001	0.0031	2.00
	1.0002	0.998	0.0022	0.0033	2.00
	1.9973	1.993	0.0043	0.0084	2.00
590	0.0000	0.000	0.0000	0.0028	2.00
	0.5517	0.552	-0.0003	0.0030	2.00
	1.0803	1.079	0.0013	0.0030	2.00
	2.0373	2.032	0.0053	0.0079	2.00
635	0.0000	0.000	0.0000	0.0028	2.00
	0.5591	0.559	0.0001	0.0031	2.00
	1.0518	1.050	0.0018	0.0030	2.00
	1.9274	1.923	0.0044	0.0079	2.00

เอกสารไม่ควบคุม

FM-708-02 R01 1/11/2021

DQE Services Co.,Ltd.
32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Bangkok 10230
Phone : +66 (0)2 538 2054, Email : dqeservicesinfo@gmail.com



REPORT OF CALIBRATION

Certificate No. : SP25-001Page 4 of 5



Photometric Accuracy :

Wavelength (nm.)	CRMs Values (Abs)	UUC Reading (Abs)	Correction (Abs)	Uncertainty (Abs)	Coverage factor k
235	0.0000	0.000	0.0000	0.0050	2.00
	0.7469	0.744	0.0029	0.0057	2.00
257	0.0000	0.000	0.0000	0.0050	2.00
	0.8674	0.863	0.0044	0.0059	2.00
313	0.0000	0.000	0.0000	0.0050	2.00
	0.2919	0.290	0.0019	0.0051	2.00
350	0.0000	0.000	0.0000	0.0050	2.00
	0.6430	0.640	0.0030	0.0055	2.00

เอกสารไม่ควบคุม

FM-708-02 R01 1/11/2021

DQE Services Co.,Ltd.
32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Bangkok 10230
Phone : +66 (0)2 538 2054, Email : dqeservicesinfo@gmail.com



REPORT OF CALIBRATION

Certificate No. : SP25-001Page 5 of 5

Wavelength Accuracy :

CRMs Values (nm.)	UUC Reading (nm.)	Correction (nm.)	Uncertainty (nm.)	Coverage factor k
241.72	241.1	0.62	0.18	2.00
279.45	279.0	0.45	0.18	2.00
287.81	287.3	0.51	0.18	2.00
334.06	333.8	0.26	0.18	2.00
360.93	360.6	0.33	0.18	2.00
418.59	418.2	0.39	0.18	2.00
445.94	445.5	0.44	0.18	2.00
453.66	453.4	0.26	0.18	2.00
460.02	459.8	0.22	0.18	2.00
536.59	536.6	-0.01	0.18	2.00
637.98	637.7	0.28	0.18	2.00
431.38	431.1	0.28	0.18	2.00
472.50	472.3	0.20	0.18	2.00
513.47	513.4	0.07	0.18	2.00
528.88	528.9	-0.02	0.18	2.00
573.17	573.3	-0.13	0.18	2.00
585.35	585.1	0.25	0.20	2.00
684.40	684.5	-0.10	0.18	2.00
740.72	741.0	-0.28	0.20	2.00
748.55	748.8	-0.25	0.18	2.00
807.03	807.3	-0.27	0.18	2.00
879.28	879.6	-0.32	0.18	2.00

เอกสารไม่ควบคุม

FM-708-02 R01 1/11/2021

DQE Services Co.,Ltd.
32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Bangkok 10230
Phone : +66 (0)2 538 2054, Email : dqeservicesinfo@gmail.com



CERTIFICATE OF CALIBRATION

Certificate No. : SP25-019Page 1 of 5

Customer : United Analyst and Engineering Consultant Co.,Ltd. (Head Office)

Address : 3 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260

Location of calibration : Instrument room (207)

Equipment : UV-Vis Spectrophotometer

Manufacturer : Agilent Technologies

Model : Cary 60

Serial No. : MY15410009

ID No. : UAE.WAT.020/2558

Received Date : 26 May 2025

Calibration Date : 26 May 2025

Issue Date : 29 May 2025

Condition Instrument : Good

Calibrated by : 
(Mr.Tanawut Rittidach)

Approved by : 
(Ms.Chonticha Sangern)

Technical Manager

Quality Manager


The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only.

The measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the DQE Services Co., Ltd.

เอกสารไม่ควบคุม

FM-708-02 R01 1/11/2021

DQE Services Co.,Ltd.
32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Bangkok 10230
Phone : +66 (0)2 538 2054, Email : dqeservicesinfo@gmail.com



REPORT OF CALIBRATION

Certificate No. : SP25-019Page 2 of 5

Environment Condition : Ambient Temperature 25 ± 5 °C
Relative humidity 55 ± 20 %RH

Calibration method : In-house method CP-01 Based on ASTM E275-08

Certified Reference Materials :

Material	Serial No.	Certificate No.	Due date
Absorbance Standard set	25760	115663	25 October 2025
Absorbance Standard set	25757	115638	25 October 2025
Wavelength Standard set	25806	115657	25 October 2025
Wavelength Standard set	25758	115665	25 October 2025

Traceability : This certification is traceable to the International System of Unit maintained at National -
Institute of Standards and Technology (NIST) through Starna Scientific Limited

Spectral Band Width of UUC : 1.5 nm.

Scan Speed of UUC : 60 nm/min



Scan Interval of UUC : 0.15 nm.

Resolution of UUC : Photometric 0.0001 Abs.
Wavelength 0.1 nm.

เอกสารไม่ควบคุม

FM-708-02 R01 1/11/2021

DQE Services Co.,Ltd.
32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Bangkok 10230
Phone : +66 (0)2 538 2054, Email : dqeservicesinfo@gmail.com



REPORT OF CALIBRATION

Certificate No. : SP25-019Page 3 of 5

Calibration Results : Without adjustment



Photometric Accuracy :

Wavelength (nm.)	CRMs Values (Abs)	UUC Reading (Abs)	Correction (Abs)	Uncertainty (Abs)	Coverage factor k
420	0.0000	0.0000	0.0000	0.0028	2.00
	0.5780	0.5739	0.0041	0.0031	2.00
	1.0484	1.0430	0.0054	0.0029	2.00
	2.1876	2.1876	0.0000	0.0084	2.00
440	0.0000	0.0000	0.0000	0.0028	2.00
	0.5595	0.5581	0.0014	0.0034	2.00
	1.0239	1.0219	0.0020	0.0035	2.00
	2.1230	2.1207	0.0023	0.0085	2.00
465	0.0000	0.0000	0.0000	0.0028	2.00
	0.5230	0.5190	0.0040	0.0029	2.00
	0.9633	0.9609	0.0024	0.0029	2.00
	1.9753	1.9719	0.0034	0.0079	2.00
546.1	0.0000	0.0000	0.0000	0.0028	2.00
	0.5181	0.5161	0.0020	0.0031	2.00
	1.0002	0.9979	0.0023	0.0033	2.00
	1.9973	2.0021	-0.0048	0.0102	2.00
590	0.0000	0.0000	0.0000	0.0028	2.00
	0.5517	0.5503	0.0014	0.0030	2.00
	1.0803	1.0808	-0.0005	0.0031	2.00
	2.0373	2.0324	0.0049	0.0105	2.00
635	0.0000	0.0000	0.0000	0.0028	2.00
	0.5591	0.5583	0.0008	0.0031	2.00
	1.0518	1.0513	0.0005	0.0030	2.00
	1.9274	1.9281	-0.0007	0.0102	2.00

เอกสารไม่ควบคุม

FM-708-02 R01 1/11/2021

DQE Services Co.,Ltd.
32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Bangkok 10230
Phone : +66 (0)2 538 2054, Email : dqeservicesinfo@gmail.com



REPORT OF CALIBRATION

Certificate No. : SP25-019Page 4 of 5



Photometric Accuracy :

Wavelength (nm.)	CRMs Values (Abs)	UUC Reading (Abs)	Correction (Abs)	Uncertainty (Abs)	Coverage factor k
235	0.0000	0.0000	0.0000	0.0050	2.00
	0.7469	0.7488	-0.0019	0.0063	2.00
257	0.0000	0.0000	0.0000	0.0050	2.00
	0.8674	0.8663	0.0011	0.0067	2.00
313	0.0000	0.0000	0.0000	0.0050	2.00
	0.2919	0.2902	0.0017	0.0052	2.00
350	0.0000	0.0000	0.0000	0.0050	2.00
	0.6430	0.6428	0.0002	0.0063	2.00

เอกสารไม่ควบคุม

FM-708-02 R01 1/11/2021

DQE Services Co.,Ltd.
32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Bangkok 10230
Phone : +66 (0)2 538 2054, Email : dqeservicesinfo@gmail.com



REPORT OF CALIBRATION

Certificate No. : SP25-019Page 5 of 5

Wavelength Accuracy :

CRMs Values (nm.)	UUC Reading (nm.)	Correction (nm.)	Uncertainty (nm.)	Coverage factor k
241.72	242.0	-0.28	0.18	2.00
279.45	279.5	-0.05	0.18	2.00
287.81	287.6	0.21	0.18	2.00
334.06	333.8	0.26	0.18	2.00
360.93	360.5	0.43	0.18	2.00
418.59	417.9	0.69	0.18	2.00
445.94	445.4	0.54	0.18	2.00
453.66	453.2	0.46	0.18	2.00
460.02	459.6	0.42	0.18	2.00
536.59	536.5	0.09	0.18	2.00
637.98	638.5	-0.52	0.18	2.00
431.38	430.7	0.68	0.18	2.00
472.50	472.3	0.20	0.18	2.00
513.47	513.5	-0.03	0.18	2.00
528.88	528.9	-0.02	0.18	2.00
573.17	573.8	-0.63	0.18	2.00
585.35	585.2	0.15	0.20	2.00
684.40	685.1	-0.70	0.18	2.00
740.72	741.1	-0.38	0.20	2.00
748.55	748.9	-0.35	0.18	2.00
807.03	807.1	-0.07	0.18	2.00
879.28	879.1	0.18	0.18	2.00

Remark : - UUC = Unit Under Calibration

- N/A = Not Available



- The result expanded uncertainty of measurement U is stated as the standard uncertainty of measurement multiplied by the coverage factor k, which for a normal distribution corresponds to a coverage probability of approximately 95%

- End of Certificate -

เอกสารไม่ควบคุม

FM-708-02 R01 1/11/2021

DQE Services Co.,Ltd.
32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Bangkok 10230
Phone : +66 (0)2 538 2054, Email : dqeservicesinfo@gmail.com



CERTIFICATE OF CALIBRATION

Certificate No. : SP25-024

Page 1 of 5

Customer : United Analyst and Engineering Consultant Co.,Ltd. (Head Office)

Address : 3 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260

Location of calibration : Instrument room (207)

Equipment : UV-Vis Spectrophotometer

Manufacturer : HITACHI

Model : U-5100

Serial No. : 23A4-008


ID No. : UAE.WAS.010/2567


Received Date : 17 June 2025

Calibration Date : 17 June 2025

Issue Date : 20 June 2025

Condition Instrument : Good

Calibrated by : 
(Mr.Tanawut Rittidach)
Technical Manager

Approved by : 
(Ms.Chonticha Sangern)
Quality Manager



The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only.

The measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the DQE Services Co., Ltd.

เอกสารไม่ควบคุม

FM-708-02 R01 1/11/2021

DQE Services Co.,Ltd.
32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Bangkok 10230
Phone : +66 (0)2 538 2054, Email : dqeservicesinfo@gmail.com



REPORT OF CALIBRATION

Certificate No. : SP25-024

Page 2 of 5

Environment Condition : Ambient Temperature 25 ± 5 °C

Relative humidity 55 ± 20 %RH

Calibration method : In-house method CP-01 Based on ASTM E275-08

Certified Reference Materials :

Material	Serial No.	Certificate No.	Due date
Absorbance Standard set	25760	115663	25 October 2025
Absorbance Standard set	25757	115638	25 October 2025
Wavelength Standard set	25806	115657	25 October 2025
Wavelength Standard set	25758	115665	25 October 2025

Traceability : This certification is traceable to the International System of Unit maintained at National -
Institute of Standards and Technology (NIST) through Starna Scientific Limited

Spectral Band Width of UUC : 5.0 nm.

Scan Speed of UUC : 40



Scan Interval of UUC : 0.1 nm.

Resolution of UUC : Photometric 0.001 Abs.
Wavelength 0.1 nm.

เอกสารไม่ควบคุม

FM-708-02 R01 1/11/2021

DQE Services Co.,Ltd.
32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Bangkok 10230
Phone : +66 (0)2 538 2054, Email : dqeservicesinfo@gmail.com



REPORT OF CALIBRATION

Certificate No. : SP25-024

Page 3 of 5

Calibration Results : Without adjustment



Photometric Accuracy :

Wavelength (nm.)	CRMs Values (Abs)	UUC Reading (Abs)	Correction (Abs)	Uncertainty (Abs)	Coverage factor k
420	0.0000	0.000	0.0000	0.0028	2.00
	0.5780	0.574	0.0040	0.0031	2.00
	1.0484	1.044	0.0044	0.0029	2.00
	2.1876	2.185	0.0026	0.0075	2.00
440	0.0000	0.000	0.0000	0.0028	2.00
	0.5595	0.558	0.0015	0.0035	2.00
	1.0239	1.021	0.0029	0.0035	2.00
	2.1230	2.122	0.0010	0.0079	2.00
465	0.0000	0.000	0.0000	0.0028	2.00
	0.5230	0.519	0.0040	0.0030	2.00
	0.9633	0.961	0.0023	0.0029	2.00
	1.9753	1.975	0.0003	0.0071	2.00
546.1	0.0000	0.000	0.0000	0.0028	2.00
	0.5181	0.515	0.0031	0.0031	2.00
	1.0002	0.996	0.0042	0.0033	2.00
	1.9973	1.994	0.0033	0.0084	2.00
590	0.0000	0.000	0.0000	0.0028	2.00
	0.5517	0.549	0.0027	0.0030	2.00
	1.0803	1.078	0.0023	0.0030	2.00
	2.0373	2.031	0.0063	0.0082	2.00
635	0.0000	0.000	0.0000	0.0028	2.00
	0.5591	0.557	0.0021	0.0031	2.00
	1.0518	1.049	0.0028	0.0030	2.00
	1.9274	1.924	0.0034	0.0081	2.00

เอกสารไม่ควบคุม

FM-708-02 R01 1/11/2021

DQE Services Co.,Ltd.
32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Bangkok 10230
Phone : +66 (0)2 538 2054, Email : dqeservicesinfo@gmail.com



REPORT OF CALIBRATION

Certificate No. : SP25-024

Page 4 of 5

Photometric Accuracy :

Wavelength (nm.)	CRMs Values (Abs)	UUC Reading (Abs)	Correction (Abs)	Uncertainty (Abs)	Coverage factor k
235	0.0000	0.000	0.0000	0.0050	2.00
	0.7469	0.747	-0.0001	0.0057	2.00
257	0.0000	0.000	0.0000	0.0050	2.00
	0.8674	0.864	0.0034	0.0059	2.00
313	0.0000	0.000	0.0000	0.0050	2.00
	0.2919	0.293	-0.0011	0.0051	2.00
350	0.0000	0.000	0.0000	0.0050	2.00
	0.6430	0.639	0.0040	0.0055	2.00

เอกสารไม่ควบคุม

FM-708-02 R01 1/11/2021

DQE Services Co.,Ltd.

DQE Services

32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Bangkok 10230

Phone : +66 (0)2 538 2054, Email : dqeservicesinfo@gmail.com

ISO 9001:2015

CALIBRATION 0004

REPORT OF CALIBRATION

Certificate No. : SP25-024

Page 5 of 5

Wavelength Accuracy :

CRMs Values (nm.)	UUC Reading (nm.)	Correction (nm.)	Uncertainty (nm.)	Coverage factor k
241.00	240.4	0.60	0.18	2.00
279.30	278.8	0.50	0.18	2.00
288.90	288.3	0.60	0.18	2.00
334.50	333.9	0.60	0.18	2.00
361.40	360.8	0.60	0.18	2.00
418.40	417.9	0.50	0.18	2.00
447.20	446.6	0.60	0.18	2.00
459.30	459.1	0.20	0.18	2.00
537.00	536.4	0.60	0.18	2.00
638.00	637.5	0.50	0.18	2.00
441.29	440.7	0.59	0.18	2.00
479.88	479.4	0.48	0.18	2.00
513.75	513.3	0.45	0.18	2.00
528.59	528.2	0.39	0.18	2.00
575.10	574.5	0.60	0.18	2.00
585.56	585.4	0.16	0.20	2.00
684.70	684.1	0.60	0.18	2.00
740.51	740.2	0.31	0.20	2.00
747.61	747.0	0.61	0.18	2.00
807.04	806.4	0.64	0.18	2.00
879.68	879.1	0.58	0.18	2.00

Remark : - UUC = Unit Under Calibration

- N/A = Not Available

- The result expanded uncertainty of measurement U is stated as the standard uncertainty of measurement multiplied by the coverage factor k ,

which for a normal distribution corresponds to a coverage probability of approximately 95%

- End of Certificate -

เอกสารไม่ควบคุม

Technology

DKSH

Service Report

TO

Company: United Analyst and Engineering Consultant Co., Ltd. _ Bangkok-HQ

Address: 700/2 หมู่ที่ 1

Phrakhanong District, Bangkok, 10260

FOR

Work Order Number: WO-00074079

Contact: Karnphong Boonpuang

Email: karnphong.b@uaeconsultant.co.th

Tel: +66 2763 2828 (7021), +66 8 6347 7390

WORK ORDER INFORMATION

Top-Level		Order Type	Preventive Maintenance
Installed Product ID	IB-00105024	Billing Type	Chargeable
Product	SKALAR 2SAN59000 SAN++ Classic CFA 230V 2SAN59000	PO No.	HPO-250400209
Serial No.	182688	Warranty No.	
		Contract No.	

PRODUCTS SERVICED

Installed Product Id	Serial Number	Product
IB-00105024	182688	SKALAR 2SAN59000 SAN++ Classic CFA 230V 2SAN59000

PROBLEM DESCRIPTION

PM 1 ครั้ง/ปี **ในแผนการเวลาเลขที่ Q-120095

Line Number	Engineer	Start Date And Time	End Date And Time	Billable Labor Hour	Billable Travel Hour	Travel KM
WL-00342192	Yongyuth Chanphong	05/23/2025 9:30 AM	05/23/2025 6:00 PM	8.5		
Total				8.5	0	0

I Reach us at DKSH Service-Hotline : +66 2 639 7000

2533 Sukhumvit Road, Bangkok, 10260, Phrakhanong, Bangkok, Thailand

Phone +66 2 639 7000 Fax +66 2 333 1026

เอกสารไม่ควบคุม

Technology

DKSH

Line Number	Work Description
WL-00342192	- ทำ PM เสร็จแล้ว, เครื่องพร้อมใช้งาน

PARTS CONSUMED

Part No	Part Description	Quantity
---------	------------------	----------

EXPENSES

Part No	Expense Type	Description	Line Quantity
---------	--------------	-------------	---------------

RECOMMENDED PARTS

อะไหล่สำรองที่ควรสั่งซื้อทั้งหมด 7 รายการ คือ Pump tube 3 รายการ (SA3028, SA3032 และ SA3034), หลอดไฟ Halogen 6V/10W (90020012) 1 รายการ จำนวน 2 หลอด, Tubing polyethylene 3 รายการ (SA3142, SA5141 และ SA5142)

REMARKS

Travel Time Disclaimer:

Please note that the travel time in this report only includes time taken to reach the installed equipment location. It does not include our engineer's return travel time.

Customer Signature:

Technician: Yongyuth Chanphong

Job Title: Service Manager

Email: yongyuth.yc@dksh.com

Customer Signature

Date: 06/06/2025

เอกสารไม่ควบคุม

Technology

DKSH

Job No. WO-00074079

Test Report

Customers

United Analyst and Engineering Consultant Co., Ltd.

Equipment	Continuous Flow Analyzer	Manufacturer	SKALAR
Controller Mdel	SA5000	Auto Sample Model	SA1052
Controller Serial No.	182688	Auto Sample Serial No.	181729
Date of test	23-May-2025	Period	12 Month
Environment temperature	24.3 °C	Humidity	54.4 %RH

Results

Instrument Checked

Item	Characteristic	Before	After	Remark
1	Visual inspect	<input checked="" type="checkbox"/> Pass <input type="checkbox"/> Fail	<input checked="" type="checkbox"/> Pass <input type="checkbox"/> Fail	
2	Power supply (210 - 240 VAC)	220 VAC	220 VAC	
3	Computer	<input checked="" type="checkbox"/> Pass <input type="checkbox"/> Fail	<input checked="" type="checkbox"/> Pass <input type="checkbox"/> Fail	
4	Program	<input checked="" type="checkbox"/> Pass <input type="checkbox"/> Fail	<input checked="" type="checkbox"/> Pass <input type="checkbox"/> Fail	
5	Auto sampler	<input checked="" type="checkbox"/> Pass <input type="checkbox"/> Fail	<input checked="" type="checkbox"/> Pass <input type="checkbox"/> Fail	
6	Module holder			
	- Motor pump	<input checked="" type="checkbox"/> Pass <input type="checkbox"/> Fail	<input checked="" type="checkbox"/> Pass <input type="checkbox"/> Fail	
	- Pump tube	<input checked="" type="checkbox"/> Pass <input type="checkbox"/> Fail	<input checked="" type="checkbox"/> Pass <input type="checkbox"/> Fail	*
	- Air-injection	<input checked="" type="checkbox"/> Pass <input type="checkbox"/> Fail	<input checked="" type="checkbox"/> Pass <input type="checkbox"/> Fail	*
	- Chemistry manifolds, Switching valve, Coil, Membrane	<input checked="" type="checkbox"/> Pass <input type="checkbox"/> Fail	<input checked="" type="checkbox"/> Pass <input type="checkbox"/> Fail	
7	Detector			
	- Filter	<input checked="" type="checkbox"/> Pass <input type="checkbox"/> Fail	<input checked="" type="checkbox"/> Pass <input type="checkbox"/> Fail	
	- Flow cell	<input checked="" type="checkbox"/> Pass <input type="checkbox"/> Fail	<input checked="" type="checkbox"/> Pass <input type="checkbox"/> Fail	
	- Lamp	<input checked="" type="checkbox"/> Pass <input type="checkbox"/> Fail	<input checked="" type="checkbox"/> Pass <input type="checkbox"/> Fail	
8	Interface	<input checked="" type="checkbox"/> Pass <input type="checkbox"/> Fail	<input checked="" type="checkbox"/> Pass <input type="checkbox"/> Fail	
9	Rinsing valves	<input checked="" type="checkbox"/> Pass <input type="checkbox"/> Fail <input type="checkbox"/> N/A	<input checked="" type="checkbox"/> Pass <input type="checkbox"/> Fail <input type="checkbox"/> N/A	
10	Temperature / Reactor	<input checked="" type="checkbox"/> Pass <input type="checkbox"/> Fail <input type="checkbox"/> N/A	<input checked="" type="checkbox"/> Pass <input type="checkbox"/> Fail <input type="checkbox"/> N/A	
11	Flame photometer	<input checked="" type="checkbox"/> Pass <input type="checkbox"/> Fail <input type="checkbox"/> N/A	<input checked="" type="checkbox"/> Pass <input type="checkbox"/> Fail <input type="checkbox"/> N/A	
12	UPS / Stabilizer	<input checked="" type="checkbox"/> Pass <input type="checkbox"/> Fail <input type="checkbox"/> N/A	<input checked="" type="checkbox"/> Pass <input type="checkbox"/> Fail <input type="checkbox"/> N/A	

Warning and Error Checked

Item	Event	Before	After
13	Error list	<input type="checkbox"/> None <input type="checkbox"/> Appear : _____	<input type="checkbox"/> None <input type="checkbox"/> Appear : _____

DKSH Technology Limited (Head office)

2533 Sukhumvit Road, Bangkok, Phrakhanong, Bangkok, 10260

Phone +66 2 639 7000, Mobile +66 93 813 8681, yongyuth.yc@dksh.com, www.dksh.com

เอกสารไม่ควบคุม

Check with Standard

Item	Characteristic	Before	After	Remark
14	Base Line Test	<input type="checkbox"/> Pass <input type="checkbox"/> Fail <input type="checkbox"/> N/A	<input type="checkbox"/> Pass <input type="checkbox"/> Fail <input type="checkbox"/> N/A	
15	Detector Signal Test	<input type="checkbox"/> Pass <input type="checkbox"/> Fail <input type="checkbox"/> N/A	<input type="checkbox"/> Pass <input type="checkbox"/> Fail <input type="checkbox"/> N/A	

Summary of checked

- ☐ The instrument can work normally and efficiently. (เครื่องมือสามารถทำงานได้ปกติและมีประสิทธิภาพ)
- ☐ The instrument can work but it's requiring to maintenance. (เครื่องมือสามารถทำงานได้แต่ต้องบำรุงรักษา)
- ☐ The instrument could not work it's requiring to repair. (เครื่องมือไม่สามารถทำงานได้แต่ต้องทำการซ่อมบำรุง)

Remark :

* Pump tube, Tubing polyethylene และ Air tube เป็นวัสดุคุณภาพ ได้รับรองจากห้องปฏิบัติการและผ่านการตรวจสอบ


หมายเหตุ และข้อมูลอ้างอิงเครื่องมือ 7 รายการ ดังนี้

1. แก๊ส Ammonia จำนวน 3 รายการ (SA3032, SA5141 และ 90020012)

2. แก๊ส Phenol และ Cyanide จำนวน 6 รายการ (SA3028, SA3034, SA3142, SA5142 และ 90020012)

Standard Equipment Used

Equipment	Equipment I.D.
Digital multi meter	S/N 57600592 Due date : 19-Jun-2025
Thermo hygrometer	S/N 39520444/904 Due date : 27-Dec-2025

Test By : 
(Mr. Yongyuth Chanphong)

Approved by : 
(Mr. Eknopong Wankiang)

Position : Supervisor, Technical Service

Position : Manager, Technical Services


DKSH Technology Limited (Head office)
2533 Sukhumvit Road, Bangkok, Phrakhanong, Bangkok, 10260
Phone +66 2 639 7000, Mobile +66 93 813 8681, yongyuth.yc@dksh.com, www.dksh.com

Delivering Growth – in Asia and Beyond

เอกสารไม่ควบคุม

Page 2/2

Base Line Test : Reagent_Baseline_CN_Phenol_NH3

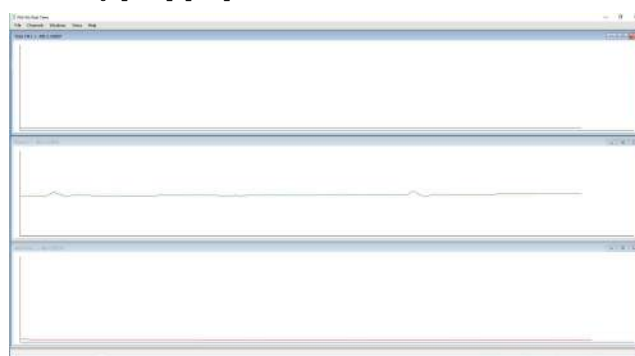



DKSH Technology Limited (Head office)
2533 Sukhumvit Road, Bangkok, Phrakhanong, Bangkok, 10260
Phone +66 2 639 7000, Mobile +66 93 813 8681, yongyuth.yc@dksh.com, www.dksh.com

Delivering Growth – in Asia and Beyond

เอกสารไม่ควบคุม

Page 3/2

Detector Signal Test : Phenol

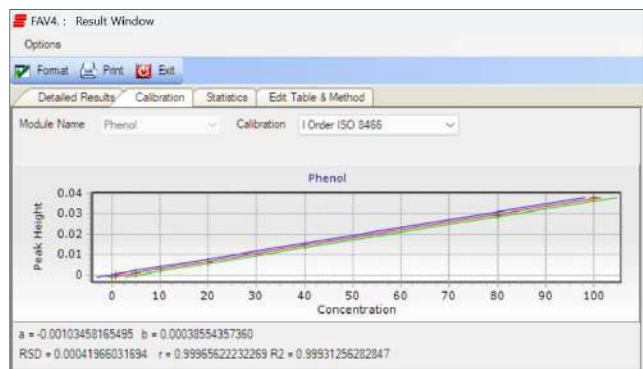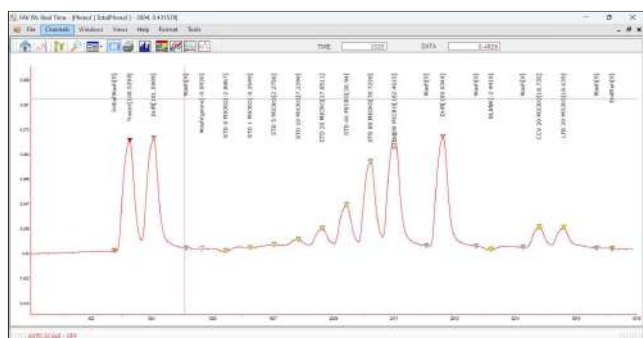



DKSH Technology Limited (Head office)
2533 Sukhumvit Road, Bangkok, Phrakhanong, Bangkok, 10260
Phone +66 2 639 7000, Mobile +66 93 813 8681, yongyuth.yc@dksh.com, www.dksh.com

Delivering Growth – in Asia and Beyond

เอกสารไม่ควบคุม

Page 4/2

Detector Signal Test : NH3

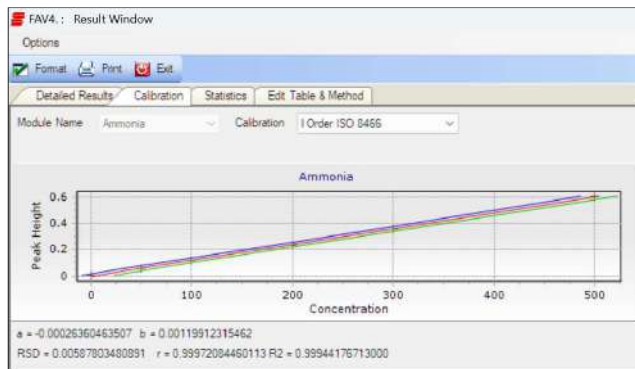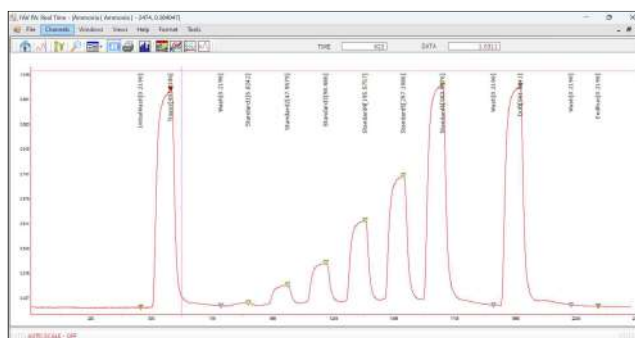



DKSH Technology Limited (Head office)
2533 Sukhumvit Road, Bangkok, Phrakhanong, Bangkok, 10260
Phone +66 2 639 7000, Mobile +66 93 813 8681, yongyuth.yc@dksh.com, www.dksh.com

Delivering Growth – in Asia and Beyond

เอกสารไม่ควบคุม

Page 5/2

Detector Signal Test : CN

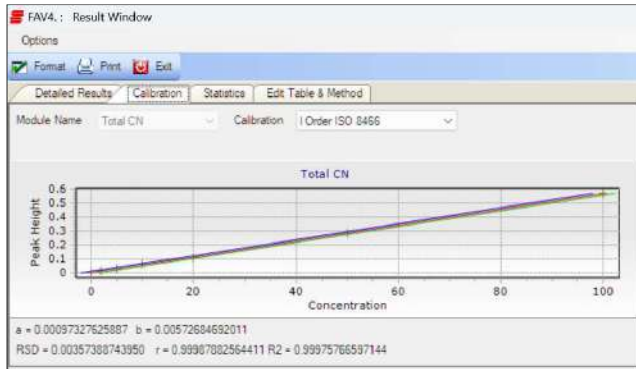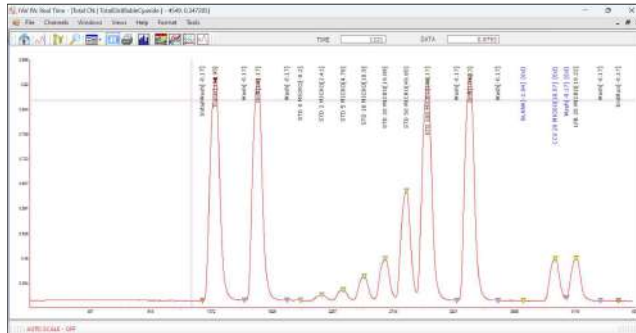

DKSH Technology Limited (Head office)
2533 Sukhumvit Road, Bangkok, Prakhong, Bangkok, 10260
Phone +66 2 639 7000, Mobile +66 93 813 8681, yongyuth.yc@dksh.com, www.dksh.com

Delivering Growth - In Asia and Beyond

เอกสารไม่ควบคุม

Page 6/2

Calibration Certificate

Certificate No.: 2502228-003-01
Client name: UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.
Address: 3 Soi Udomsuk 41, Sukhumvit Road,
Bangchack, Prakhong, Bangkok 10260

Page 1 of 3

Equipment: Electronic Balance
Manufacturer: METTLER TOLEDO
Model: MS204TS/00
Serial No.: C252436235
ID No.: UAE.AIR.023/2566
Order No.: 2502228
Operation No.: 2502228-003
Date of Receipt: 19 March 2025
Date of Calibration: 19 March 2025

Calibrated by Mr.Yothin Charoensuk Scientist
Approved by *N. Niyodatt* (Mr.Pheraphat Tuanjit)
Manager, Division of Calibration Laboratory
Responsible for the Technical Management Team
Date of Issue: 25 March 2025

The uncertainties are for a confidence probability of approximately 95%

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the National Food Institute.

FCS-009 Revision: 01 Date: 20-04-65

เอกสารไม่ควบคุม

Calibration Report

Certificate No.: 2502228-003-01
Equipment: Electronic Balance
Manufacturer: METTLER TOLEDO
Model: MS204TS/00
Resolution: 0.0001 g
Serial No.: C252436235
ID No.: UAE.AIR.023/2566
Capacity: 220 g

Date of Calibration: 19 March 2025 Page 2 of 3

Environment Condition: Ambient Temperature: 21.1 ± 0.6 °C Relative Humidity: 55 ± 0.75 %

Place of Calibration: 206 Balance Room 2, UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.

Condition of Equipment: Good Condition

Condition of This Results of Calibration:

1. Calibration Method: NFI Method W-MA-001 In-House Method based on UKAS Lab 14 : 2019

2. Reference Standards:

Reference Standard Model Serial No. Calibrated By Certificate No. Due Date
Standard Weight Class E2 1mg to 200g 8505567572 TCS M24041005 19 April 2025

Instrument Model Serial No. Calibrated By Certificate No. Due Date
Thermo-Hygro Meter 608-H1 NFI.BTH 017/23 Quality Reborn QR25-0542 10 February 2026

3. This certification is traceable to SI UNIT

4. This certificate was certified only for the instrument we calibrated.

5. This result of calibration was found accurate as shown on date and place of calibration only.

Calibration Results:


1. Repeatability of Reading:

Nominal Value (g)	Standard Deviation of Reading (g)
100	0.000052
200	0.000079

2. Off-Center Error:

A mass of 200 g was placed and moved to various position on pan.

The balance reading obtained is given in the table.



1	2	3	4	5	6	(Maximum Difference)
(g)	(g)	(g)	(g)	(g)	(g)	(g)
99.9997	99.9995	99.9995	99.9997	99.9999	99.9998	0.0003

FCS-012 Revision: 01 Date: 20-04-65

เอกสารไม่ควบคุม

เอกสารไม่ควบคุม

Calibration Report

Certificate No.: 2502228-003-01
Equipment: Electronic Balance
Manufacturer: METTLER TOLEDO
Model: MS204TS/00
Resolution: 0.0001 g
Serial No.: C252436235
ID No.: UAE.AIR.023/2566
Capacity: 220 g

Date of Calibration: 19 March 2025 Page 3 of 3

Calibration Results: (Continued)

Calibration Range: 0-200 g

Calibration Adjustment: Internal Calibration

3. Departure from Nominal Value:

Nominal Value (g)	Standard Value (g)	Average Reading (g)	Correction (g)	Uncertainty (±g)	Coverage Factor
Unloaded	0.00000	0.00000	0.00000	0.000089	2.00
0.1	0.10001	0.10001	-0.00001	0.000089	2.00
1	1.00000	1.00000	0.00000	0.000089	2.00
3	3.00003	3.00000	0.00000	0.000091	2.00
5	5.00002	5.00000	0.00000	0.000090	2.00
10	10.00001	9.99999	0.00001	0.000092	2.00
20	20.00003	20.00000	0.00000	0.000096	2.00
50	50.00003	49.99998	0.00002	0.000012	2.00
70	70.00005	69.99998	0.00003	0.000013	2.00
100	100.00006	99.99998	0.00003	0.000016	2.00
150	150.00009	150.00000	0.00001	0.000021	2.00
200	200.00013	200.00000	0.00001	0.000029	2.00

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k, providing a level of confidence of approximately 95 %.

----- End -----

FCS-012 Revision: 01 Date: 20-04-65

เอกสารไม่ควบคุม

เอกสารไม่ควบคุม

List of Instruments Certification for Air & Noise Quality Analysis

No.	Instrument/Equipment	Parameter	Manufacturer	Model/Serial No.	Calibrator	Certification No.	Date of Calibration	Due date of Calibration	Remark
Ambient									
1	Orifice Transfer Standard Calibrator	Total Suspended Particulate (TSP) Particulate Matter < 10 µm (PM ₁₀)	Tisch Environmental,Inc.	TE-5025A 3540	Jiranatee Associates Co., Ltd.	COF-045-67	4 Nov 24	3 Nov 25	-
2	U-Tube Manometer	Total Suspended Particulate (TSP) Particulate Matter < 10 µm (PM ₁₀)	Dwyer	1221-36-W/M -	Technology Promotion Association (Thailand-Japan)	25P1538	25 Apr 25	24 Apr 26	-
3	Aneroid Barometer	Total Suspended Particulate (TSP) Particulate Matter < 10 µm (PM ₁₀)	Barigo, Germany	-	Technology Promotion Association (Thailand-Japan)	25P1376	17 Apr 25	16 Apr 26	-
4	Dial Thermo-Hygrometer	Total Suspended Particulate (TSP) Particulate Matter < 10 µm (PM ₁₀)	Barigo, Germany	-	Technology Promotion Association (Thailand-Japan)	25H807	10 Apr 25	9 Apr 26	-
5	Nitrogen Dioxide Analyzer	Nitrogen Dioxide	Thermo Environmental Instrument	42C 42C-78933-390	UAE Consultant Co.,Ltd.	07052025	7 May 25	6 May 26	-
6	Nitrogen Dioxide Analyzer	Nitrogen Dioxide	Thermo Scientific	42i 1180540063	UAE Consultant Co.,Ltd.	02052025	2 May 25	1 May 26	-
7	Nitrogen Dioxide Analyzer	Nitrogen Dioxide	Thermo Scientific	42i 1182920005	UAE Consultant Co.,Ltd.	07052025	7 May 25	6 May 26	-
8	Standard Gases (Mixture)	Nitrogen Dioxide	Airgas	EB0162121 2016PSIG	Airgas an Air Liquide company	E05NI91E15A0014	6 Jun 23	6 Jun 31	-
9	Sulphur Dioxide Analyzer	Sulphur Dioxide	Thermo Scientific	43i CM22387067	UAE Consultant Co.,Ltd.	06052025	6 May 25	5 May 26	-
10	Sulphur Dioxide Analyzer	Sulphur Dioxide	Thermo Scientific	43i 1182920017	UAE Consultant Co.,Ltd.	07052025	6 May 25	5 May 26	-
11	Sulphur Dioxide Analyzer	Sulphur Dioxide	Thermo Scientific	43i 1180540065	UAE Consultant Co.,Ltd.	12052025	12 May 25	11 May 26	-
12	Standard Gases (Mixture)	Sulphur Dioxide	Airgas	EB0162121 2016PSIG	Airgas an Air Liquide company	E05NI91E15A0014	6 Jun 23	6 Jun 31	-
13	Wind Speed/Wind Direction	WS/WD	Met One Instument	466A / 034B X4726 / N3282	Thai Meteorological Department	215/25	14 Apr 25	13 Apr 26	-
14	Sound Level Calibrator (Acoustic Calibrator)	Calibrate Sound Level Meter	Larson Davis	CAL200 21091	Innovative Instrument Co.,Ltd.	25-ACT-074	20 May 25	19 May 26	-

List of Instruments Certification for Air & Noise Quality Analysis

No.	Instrument/Equipment	Parameter	Manufacturer	Model/Serial No.	Calibrator	Certification No.	Date of Calibration	Due date of Calibration	Remark
Ambient									
15	Sound Level Meter	L _{Aeq} 24 hrs, L _{Aeq} 1 hr, L _{Amax} , L _{A90} , L _{Adn}	Larson Davis	LxT1	Electrical And Electronics Institute Foundation For Industrial Development	CP20240324EA	22 Aug 24	21 Aug 26	-
		Annoyance Noise		0007302					
16	Sound Level Meter	L _{Aeq} 24 hrs, L _{Aeq} 1 hr, L _{Amax} , L _{A90} , L _{Adn}	Larson Davis	LxT1	Electrical And Electronics Institute Foundation For Industrial Development	CP2020339EA	20 Sep 24	19 Sep 26	-
		Annoyance Noise		0007303					
17	Sound Level Meter	L _{Aeq} 24 hrs, L _{Aeq} 1 hr, L _{Amax} , L _{A90} , L _{Adn}	Larson Davis	LxT1	Electrical And Electronics Institute Foundation For Industrial Development	CP20240340EA	20 Sep 24	19 Sep 26	-
		Annoyance Noise		0007304					
18	Sound Level Meter	L _{Aeq} 24 hrs, L _{Aeq} 1 hr, L _{Amax} , L _{A90} , L _{Adn}	Larson Davis	LxT1	Electrical And Electronics Institute Foundation For Industrial Development	CP20240323EA	22 Aug 24	21 Aug 26	-
		Annoyance Noise		0007305					
19	Sound Level Meter	L _{Aeq} 24 hrs, L _{Aeq} 1 hr, L _{Amax} , L _{A90} , L _{Adn}	Larson Davis	LxT1	Electrical And Electronics Institute Foundation For Industrial Development	CP20240290EA	5 Aug 24	4 Aug 26	-
		Annoyance Noise		0007306					
20	Sound Level Meter	L _{Aeq} 24 hrs, L _{Aeq} 1 hr, L _{Amax} , L _{A90} , L _{Adn}	Larson Davis	LxT1	Electrical And Electronics Institute Foundation For Industrial Development	CP20240322EA	22 Aug 24	21 Aug 26	-
		Annoyance Noise		0007308					

List of Instruments Certification for Water Quality Analysis

No.	Instrument/Equipment	Parameter	Manufacturer	Model/Serial No.	Calibrator	Certification No.	Date of Calibration	Due date of Calibration	Remark
Water									
1	pH Meter	pH	Ecosence	pH100A 24H005160JEN	Technology Promotion Association (Thailand-Japan)	24CH1422	14 Nov 24	13 Nov 25	-
2	DO Meter	DO	Horiba	LAQUA-DO210 HE0L0004	Technology Promotion Association (Thailand-Japan)	24TW241	6 Dec 24	5 Dec 25	-
3	Conductivity Meter	Conductivity	YSI	Pro 30 24J101890	Technology Promotion Association (Thailand-Japan)	24CH1524	6 Dec 24	5 Dec 25	-

List of Instruments Certification for Air & Noise Quality Analysis

No.	Instrument/Equipment	Parameter	Manufacturer	Model/Serial No.	Calibrator	Certification No.	Date of Calibration	Due date of Calibration	Remark
Workplace									
1	Sound Level Calibrator (Acoustic Calibrator)	Calibrate Sound Level Meter	Larson Davis	CAL150 6458	Innovative Instrument Co.,Ltd.	25-ACT-073	20 May 25	19 May 26	-
2	Sound Level Meter	L _{Aeq} 8 hrs, L _{Amax}	Rion, Japan	NL-42 00408982	Sithiporn Associates Co., Ltd.	ACL25022	13 Jan 25	12 Jan 26	-
3	Sound Level Meter	L _{Aeq} 8 hrs, L _{Amax}	Rion, Japan	NL-42 00408983	Innovative Instrument Co.,Ltd.	25-SLM-108	18 Mar 25	17 Mar 26	-
4	Sound Level Meter	L _{Aeq} 8 hrs, L _{Amax}	Rion, Japan	NL-42 00409023	Sithiporn Associates Co., Ltd.	ACL25230	10 Jun 25	9 Jun 26	-

CERTIFICATE OF CALIBRATION

Certificate No. : CDF-045-07

Page 2 of 2 Pages

MEASUREMENT ITEM
MANUFACTURER : TISOH
MODEL/TYPE : TE-5025A
SERIAL NUMBER : 3540
ID NUMBER : UAE.EFM.176/2561
CONDITION AS-RECEIVED : Used Item
CUSTOMER : United Analyst and Engineering Consultant Co., Ltd.
81 Soi Udomsuk 41, Sukhumvit Road, Bangkok, Phrakhanong, Bangkok 10260

Calibration procedure:
The Orifice gas flow device was calibrated against Standard Rotary Displacement Meter (Roto Meter) Model G65/MC/W2-dp. The WP-CL-00M was used as a calibration guideline.

Traceability:
This certificate provides a traceability of the measurement to recognized the national standards and to realization of the international system of units (SI) through the NIMT (National Metrology Institute of Thailand) via Certificate number: M90863-21.

Uncertainty of Measurement:
The reported uncertainty of measurement is based on the standard uncertainty multiplied by a coverage factor $k=2$, which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty has been determined in accordance with the GUM "Evaluation of measurement data - Guide to the expression of uncertainty in measurement".

ENVIRONMENTAL CONDITIONS:
Ambient condition in the laboratory are as follow:
Temperature : 23.0 ± 0.5 °C
Relative Humidity : 55.0 ± 15.0 %RH
Atmospheric Pressure : 1010 ± 10 hPa

CALIBRATION CONDITION:
Preconditioning : 24 hours at ambient conditions.
Measurement Condition : The average values during measurement are 23.7 °C and 49.7 %RH.

NOTED: The certificate is valid only to the item calibrated on date and place of calibration.

TABULATION OF RESULTS:
The table on next page give the measured values.

Table 1: The results of Q standard calibration data

Plate	Flow rate m^3/min	Pressure [Pa] mmHg	Temperature [Ta] °C	Temperature [Tm] °C	Δp_{meter} mmHg	$\Delta p_{Orifice}$ mmHg	Y	Standard Flow [Qs] m^3/min
3	0.702	755.241	23.67	22.27	57.834	1.612	1.288	0.651
2	1.000	755.312	23.55	22.71	61.321	1.248	1.801	0.920
7	1.117	755.324	23.36	22.72	41.180	4.309	1.301	1.058
4	1.163	755.361	23.37	22.77	30.028	4.806	1.374	1.119
5	1.417	755.397	23.85	23.10	26.199	7.191	1.481	1.365

Slope (m): 1.98270
Intercept (b): -0.02316
Correlation coefficient (r): 0.99988
Uncertainty (k=2): 0.015 m^3/min

Table 2: The results of Q actual calibration data

Plate	Flow rate m^3/min	Pressure [Pa] mmHg	Temperature [Ta] °C	Temperature [Tm] °C	Δp_{meter} mmHg	$\Delta p_{Orifice}$ mmHg	Y	Standard Flow [Qs] m^3/min
1	0.702	755.241	23.67	22.27	57.834	1.612	0.796	0.651
2	1.000	755.312	23.55	22.71	61.321	1.248	1.129	0.920
3	1.117	755.324	23.36	22.72	41.180	4.309	1.301	1.058
4	1.163	755.361	23.37	22.77	30.028	4.806	1.374	1.119
5	1.417	755.397	23.85	23.10	26.199	7.191	1.481	1.365

Slope (m): 1.24186
Intercept (b): -0.01454
Correlation coefficient (r): 0.99988
Uncertainty (k=2): 0.015 m^3/min

End of Certificate of Calibration

Calibrated by:
☐ Mr. Suwanet Thachulad
57 Mitthitrasorn Lertratanol



Approved signatory:
Mr. Parinya Booncharoen
Calibration Department Manager



THIS CERTIFICATE REPORT MAY NOT BE REPRODUCED EXCEPT IN FULL UNLESS PERMISSION FOR REPRODUCTION HAS BEEN OBTAINED IN WRITING FROM THE LABORATORY

เอกสารไม่ควบคุม

เอกสารไม่ควบคุม



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
334/4 PATTANAKARN ROAD SOI 18, SUANLIANG, SUANLIANG, BANGKOK 10250
TEL. 0-2717-3050-24 FAX. 0-2719-9484

Certificate of Calibration

Certificate No.: 25P1538
Page: 1 of 2

Equipment : U Tube Manometer
Manufacturer: Dwyer
Model : 1221-36-W/M
Serial No.: -
ID No.: UAE.EMA2.094/2555
Condition As-Received: Used Item
Received Date: 04 April 2025
Calibration Date: 26 April 2025
Reference: 2504-0192WSC
Ambient Temperature: (23 ± 2) °C
Relative Humidity: (60 ± 15) %
Atmospheric Pressure: 1007 mbar
Submitted by: United Analyst and Engineering Consultant Co., Ltd.
81 Soi Udomsuk 41, Sukhumvit Road, Bangkok, Phrakhanong, Bangkok 10260

Procedure used: The calibration was conducted by direct comparison method against Pressure Measuring Instruments Standard according to calibration procedure CP-P04, using "DKD-R 6-1; Calibration of Pressure Gauges" as a guidelines.

Condition of this result of calibration

1. Reference standards instruments :

Instrument	Model	Serial No.	Certificate No.	Due Date
1) Pressure Calibrator	PC106P	1189	MP-0216-24	24 Sep 2025

2. This result of calibration was made on requested at the point specified by customer.

3. Scale and conversion factor is 1 kPa = 4.01463293 inHgD

4. This instrument was used clean air as pressure media.

5. This instrument was calibrated by applied pressure to high-port (+) side and low-port (-) side open to atmospheric pressure.

6. This instrument was installed in vertical orientation and top of the pressure port was used as the reference level.

7. The certificate is valid only to the item calibrated on date and place of calibration.

8. This Certification is traceable to the International System of Unit maintained through-

-National Institute of Metrology (Thailand), NSC-ONSC Accredited No. Calibration 0144

Calibrated by : Suksan Khankaw
Issue Date : 28 April 2025

Approved Signatory : Attapol P.
[] Phalinee Pratsapaipal
[] Sura Suwananari
[✓] Attapol Panurach

เอกสารไม่ควบคุม



Result of calibration: Without adjustment
Function: Pressure Measurement
Increasing Pressure

Ranges: 0 inHgD to 36 inHgD
Scale Interval: 0.1 inHgD (The Second Estimate)

Applied Pressure	High-port side	UUC Indication Low-port side	Δp	Error
0.00	0.00	0.00	0.00	0.00
2.00	1.00	-1.00	2.00	0.00
4.00	2.00	-2.00	4.00	0.00
6.00	3.00	-3.00	6.00	0.00
8.00	4.00	-4.00	8.00	0.00
10.00	5.00	-5.00	10.00	0.00
12.00	6.00	-6.00	12.00	0.00
14.00	7.00	-7.00	14.00	0.00
16.00	8.00	-8.00	16.00	0.00
18.00	9.00	-9.00	18.00	0.05
20.00	10.00	-10.00	20.00	0.05
22.00	11.00	-11.00	22.00	0.05
24.00	12.00	-12.00	24.10	0.10
26.00	13.00	-13.10	26.15	0.15
28.00	14.00	-14.10	28.15	0.15
30.00	15.00	-15.10	30.10	0.10
32.00	16.00	-16.10	32.10	0.10
34.00	17.00	-17.15	34.15	0.15
35.70	17.90	-18.00	35.90	0.20

The uncertainty of measurement was ± 0.11 inHgD

* Δp = High-port side - Low-port side

* UUC = Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k=2$, providing a level of confidence of approximately 95 %.

-0-0-

Cert.No.: 25P1538
Page: 2 of 2

เอกสารไม่ควบคุม



Certificate of Calibration

Certificate No.: 25P1376
Page: 1 of 2

Equipment: Aneroid Barometer
Manufacturer: Barigo
Model: -
Serial No.: -
ID No.: UAE/ANV.012/2547

This certificate may not be reproduced other than in full,
except with the prior written approval of the head of
Corporate Services 3: Equipment Calibration and Testing Services.

Condition As-Received: Used item
Received Date: 04 April 2025
Calibration Date: 17 April 2025

Reference: 2504-0196WSC
Ambient Temperature: $(23 \pm 2) ^\circ\text{C}$
Relative Humidity: $(50 \pm 15) \%$
Atmospheric Pressure: 1006 mbar

Submitted by: United Analyst and Engineering Consultant Co., Ltd.
81 Soi Udomsuk 41, Sukhumvit Road, Bangchak,
Phra Khanong, Bangkok 10260

Procedure used: The calibration was conducted by direct comparison method against Pressure Measuring Instruments
Standard according to calibration procedure CP-P10, using "DKD-R 6-1; Calibration of Pressure Gauges" as
a guidelines.

Condition of this result of calibration

1. Reference standards instruments:

Instrument	Model	Serial No.	Certificate No.	Due Date
1) Standard Barometer	DPI142	1422505046	MP-0133-24	15 May 2025

2. This instrument was installed in vertical orientation and center of the dial was used as the reference level.

3. This result of calibration was made on requested at the point specified by customer.

4. Scale and conversion factor is 1 kPa = 7,50062 mmHg

5. This result of calibration instrument was in absolute pressure.

6. This instrument was used clean air as pressure media.

7. The certificate is valid only to the item calibrated on date and place of calibration.

8. This Certification is traceable to the International System of Unit maintained through:-

-National Institute of Metrology Thailand (NIMT)

Calibrated by: Kaekpon Saivichai
Issue Date: 21 April 2025

Approved Signatory: Athapol P.
[] Phalinee Prabpalap
[] Sura Suwanaseri
[x] Athapol Panurath

เอกสารไม่ควบคุม



Cert.No.: 25P1376
Page: 2 of 2

Result of calibration: Without adjustment
Function: Absolute Pressure Measurement

Range: 720 mmHg to 780 mmHg
Scale Interval: 1 mmHg (The Fifth Estimate)

Increasing Pressure

Applied Pressure (mmHg)	716.79	731.30	741.30	750.93	761.77	772.78	784.62
UUC* Indication (mmHg)	720.0	730.0	740.0	750.0	760.0	770.0	780.0
Error (mmHg)	0.21	-1.30	-1.39	-0.93	-1.77	-2.78	-4.62

Decreasing Pressure

Applied Pressure (mmHg)	784.62	772.81	761.66	751.06	741.15	731.05	720.74
UUC* Indication (mmHg)	780.0	770.0	760.0	750.0	740.0	730.0	720.0
Error (mmHg)	-4.62	-2.81	-1.66	-1.06	-1.15	-1.05	-0.74

The uncertainty of measurement was ± 0.24 mmHg

* UUC = Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied
by a coverage factor $k = 2$, providing a level of confidence of approximately 95%.

-000-

เอกสารไม่ควบคุม



Certificate of Calibration

Certificate No.: 25H807
Page: 1 of 2

Equipment: Dial Thermo-Hygrometer
Manufacturer: Barigo
Model: -
Serial No.: -
ID No.: UAE/ANV.003/2548

This certificate may not be reproduced other than in full,
except with the prior written approval of the head of
Corporate Services 3: Equipment Calibration and Testing Services.

Condition As-Received: Used item
Received Date: 04 April 2025
Calibration Date: 10 April 2025
to 17 April 2025

Reference: 2504-0193WSC
Ambient Temperature: $(25 \pm 3) ^\circ\text{C}$
Relative Humidity: $(50 \pm 20) \%$

Submitted by: United Analyst and Engineering Consultant Co., Ltd.
81 Soi Udomsuk 41, Sukhumvit Road, Bangchak,
Phra Khanong, Bangkok 10260

Procedure used: Calibration were conducted using in-house calibration procedure CP-H02 according to comparison
with standard chilled mirror sensor for humidity measurement function and comparison with standard
temperature probe for temperature measurement function into humidity / temperature chamber.

Condition of this result of calibration

1. Reference standards instruments:

Instrument	Model	Serial No.	Certificate No.	Due Date
1) Chilled Mirror Hygrometer	Dew Master	44730	22688	10 Sep 2025
2) Handheld Thermometer With Sensor	1521	A5A339	241176	25 Oct 2025

2. The certificate is valid only to the item calibrated on date and place of calibration.

3. This Certification is traceable to the International System of Unit maintained through:-

-Thunder Scientific Corporation, NVLAB Accreditation No. Calibration 200562-0

-Technology Promotion Association (Thailand-Japan), NSC-ONSAC Accredited No. Calibration 0008

Calibrated by: Kaekpon Onrat
Issue Date: 21 April 2025

Approved Signatory: Viporn
[] Chakrit Waeewarjua
[] Pornthippa Taneyakul
[x] Viporn Tanayawutti

เอกสารไม่ควบคุม



Cert. No.: 25H807
Page: 2 of 2

Result of Calibration: Without Adjustment
Function: Humidity Measurement

Reference Temperature ($^{\circ}\text{C}$)	Standard Humidity (%R.H.)	UUC* Reading (%R.H.)	Correction (%R.H.)	Uncertainty of Measurement ($\pm\%$ R.H.)
25.0	40.1	39	1.1	1.7
25.0	60.0	60	0.0	1.8
25.0	80.0	79	1.0	1.9

Result of Calibration: Without Adjustment
Function: Temperature Measurement

Standard Temperature ($^{\circ}\text{C}$)	UUC* Reading ($^{\circ}\text{C}$)	Correction ($^{\circ}\text{C}$)	Uncertainty of Measurement ($\pm^{\circ}\text{C}$)
20.012	20.0	0.012	0.72
25.034	25.0	0.034	0.72
30.032	30.0	0.032	0.72
35.022	34.5	0.522	0.72
40.040	40.0	0.040	0.72

UUC* : Unit Under Calibration

The reported uncertainty of measurement was base on standard uncertainty multiplied
by coverage factor $k = 2.00$, providing confidence level approximately 95%.

-000-

เอกสารไม่ควบคุม

MULTI-POINT GAS TEST REPORT

Test Date : May 7, 2025


Equipment : Gas Analyzer (NO₂) Model : 42C
Manufacturer : Thermo Environmental Instruments Serial Number : 42C-78933-390

Standard Gas Concentration

Sulphur Dioxide (SO ₂)	42.89	PPM	Manufacturer :	Thermo Scientific
Nitric Oxide (NO)	46.77	PPM	Model :	146i
Methane (CH ₄)	-	PPM	Serial Number :	1180540071
Carbon Monoxide (CO)	965.9			
Cylinder No. :	EB0159156			
Expiration Date :	Nov 6, 2026			

Multi-point gas test data

Reference Value (ppb)	Analyzer Display (ppb)	Difference Error	Percent Error	[% Error]
Level 1 Zero	0.0	0.00	0.00	0.00
Level 2 20.00%	100.3	0.30	0.30	0.30
Level 3 40.00%	201.1	1.10	0.55	0.55
Level 4 60.00%	300.9	0.90	0.30	0.30
Level 5 80.00%	400.0	0.00	0.00	0.00
Remark : Measuring Range	500.0 ppb	Average Difference (%)	0.23	
:Acceptable Limit $\pm 5\%$				

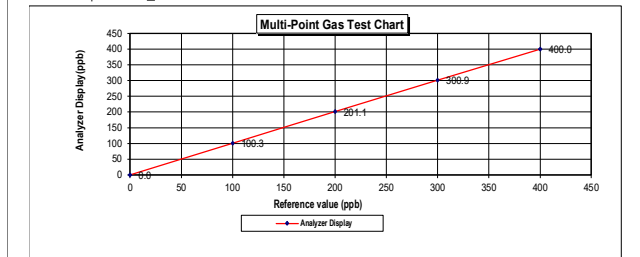

Calculate by *Sirchai S.* Approve by *Ratana R.*
7 / 05 / 2025 7 / May / 2025

MULTI-POINT GAS TEST REPORT

Test Date : May 2, 2025


Equipment : Gas Analyzer (NO₂) Model : 42i
Manufacturer : Thermo Scientific Serial Number : 1180540063

Standard Gas Concentration

Sulphur Dioxide (SO ₂)	42.89	PPM	Manufacturer :	Thermo Scientific
Nitric Oxide (NO)	46.77	PPM	Model :	146i
Methane (CH ₄)	-	PPM	Serial Number :	1180540071
Carbon Monoxide (CO)	965.9			
Cylinder No. :	EB0159156			
Expiration Date :	Nov 6, 2026			

Multi-point gas test data

Reference Value (ppb)	Analyzer Display (ppb)	Difference Error	Percent Error	[% Error]
Level 1 Zero	0.0	0.00	0.00	0.00
Level 2 20.00%	100.8	0.80	0.79	0.79
Level 3 40.00%	201.3	1.30	0.65	0.65
Level 4 60.00%	300.7	0.70	0.23	0.23
Level 5 80.00%	400.0	0.00	0.00	0.00
Remark : Measuring Range	500.0 ppb	Average Difference (%)	0.33	
:Acceptable Limit $\pm 5\%$				

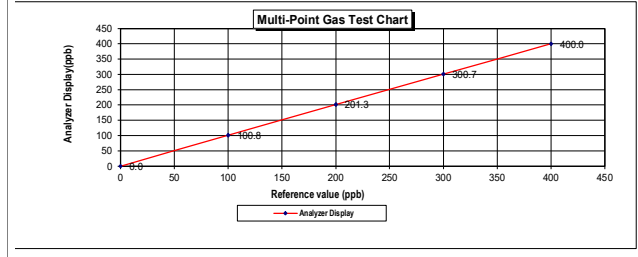

Calculate by *Sirchai S.* Approve by *Ratana R.*
2 / 05 / 2025 2 / May / 2025

MULTI-POINT GAS TEST REPORT

Test Date : May 7, 2025


Equipment : Gas Analyzer (NO₂) Model : 42i
Manufacturer : Thermo Scientific Serial Number : 1182920005

Standard Gas Concentration

Sulphur Dioxide (SO ₂)	42.89	PPM	Manufacturer :	Thermo Scientific
Nitric Oxide (NO)	46.77	PPM	Model :	146i
Methane (CH ₄)	-	PPM	Serial Number :	1180540071
Carbon Monoxide (CO)	965.9			
Cylinder No. :	EB0159156			
Expiration Date :	Nov 6, 2026			

Multi-point gas test data

Reference Value (ppb)	Analyzer Display (ppb)	Difference Error	Percent Error	[% Error]
Level 1 Zero	0.0	0.00	0.00	0.00
Level 2 20.00%	100.5	0.50	0.50	0.50
Level 3 40.00%	200.3	0.30	0.15	0.15
Level 4 60.00%	300.9	0.90	0.30	0.30
Level 5 80.00%	400.0	0.00	0.00	0.00
Remark : Measuring Range	500.0 ppb	Average Difference (%)	0.19	
:Acceptable Limit $\pm 5\%$				

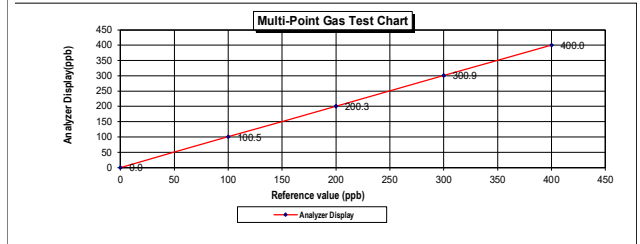

Calculate by *Sirchai S.* Approve by *Ratana R.*
7 / 05 / 2025 7 / May / 2025

CERTIFICATE OF ANALYSIS

Grade of Product: EPA PROTOCOL STANDARD

Customer: AIR LIQUIDE (THAILAND) LTD--
Part Number: E05N191E15A0014
Cylinder Number: EB0162121
Laboratory: 124 - Plumsteadville - PA
PGVP Number: A12023
Gas Code: CO, CO₂, NO, NO₂, SO₂, BALN

Reference Number: 160-402772205-1
Cylinder Volume: 144.0 CF
Cylinder Pressure: 2015 PSIG
Valve Outlet: 660
Certification Date: Jul 06, 2023
Expiration Date: Jul 06, 2031

Certification performed in accordance with EPA Traceability Protocol for Assay and Certification of Gaseous Calibration Standards (May 2012) document EPA 820-R-12-051, using the assay procedures listed. Analytical Methodology does not require correction for analytical interference. This cylinder has a total analytical uncertainty as stated below with a confidence level of 95%. There are no significant impurities which affect the use of this calibration mixture. All concentrations are on a mole/mole basis unless otherwise noted. The results relate only to the items tested. The report shall not be reproduced except in full without approval of the laboratory. Do Not Use This Cylinder below 100 psig, i.e. 3.7 megapascals.

ANALYTICAL RESULTS					
Component	Requested Concentration	Actual Concentration	Protocol Method	Total Relative Uncertainty	Assay Dates
NOX	100.0 PPM	100.4 PPM	G1	$\pm 0.9\%$ NIST Traceable	06/27/2023, 07/06/2023
NITRIC OXIDE	100.0 PPM	100.2 PPM	G1	$\pm 0.9\%$ NIST Traceable	06/27/2023, 07/06/2023
SULFUR DIOXIDE	100.0 PPM	100.5 PPM	G1	$\pm 1.4\%$ NIST Traceable	06/27/2023, 07/06/2023
CARBON MONOXIDE	200.0 PPM	199.2 PPM	G1	$\pm 0.3\%$ NIST Traceable	06/26/2023
CARBON DIOXIDE	8,000 %	7,982 %	G1	$\pm 1.3\%$ NIST Traceable	06/27/2023
NITROGEN	Balance				

CALIBRATION STANDARDS					
Type	Lot ID	Cylinder No	Concentration	Uncertainty	Expiration Date
GMIS	104202308	CC754364	98.36 PPM NITRIC OXIDE/NITROGEN	$\pm 0.4\%$	Jan 04, 2031
PRM	C2219101	AP15154048	100.16 PPM NITRIC OXIDE/NITROGEN	$\pm 0.3\%$	Feb 28, 2025
GMIS	2023042525	CC754361	98.62 PPM NITRIC OXIDE/NITROGEN	$\pm 0.4\%$	Apr 25, 2031
PRM	12409	D913860	15.01 PPM NITROGEN DIOXIDE/AIR	$\pm 1.5\%$	Feb 17, 2023
GMIS	1534002602	EB0130037	9.893 PPM NITROGEN DIOXIDE/NITROGEN	$\pm 1.0\%$	Sep 29, 2025
NTRM	160102-22	KAL203620	97.69 PPM SULFUR DIOXIDE/NITROGEN	$\pm 0.8\%$	Nov 01, 2027
CO	230801	CC745902	249.47 PPM CARBON MONOXIDE/NITROGEN	$\pm 0.3\%$	Dec 09, 2028
NTRM	130605-02	CC411730	13.359 % CARBON DIOXIDE/NITROGEN	$\pm 0.5\%$	May 14, 2025
The SRM, NTRM, PRM, or RSM noted above is only in reference to the GMIS used in the assay and not part of the analysis.					

ANALYTICAL EQUIPMENT		
Instrument/Make/Model	Analytical Principle	Last Multipoint Calibration
Nicolet iS65 FTIR AUP2010245 CO2	FTIR	Jun 15, 2023
SIEMENS ULTRAMATE6E N1-CR-180	NDIR	Jun 14, 2023
Nicolet iS55 FTIR AUP2010245 NO	FTIR	Jun 29, 2023
Nicolet iS55 FTIR AUP2010245 NO2	FTIR	Jun 15, 2023
Nicolet iS55 FTIR AUP2010245 SO2	FTIR	Jun 08, 2023

Approved for Release

MULTI-POINT GAS TEST REPORT

Test Date : May 6, 2025


Equipment : Gas Analyzer (SO₂) Model : 43i
Manufacturer : Thermo SCIENTIFIC Serial Number : CM22387067

Standard Gas Concentration

Sulphur Dioxide (SO ₂)	42.89	PPM	Manufacturer :	Thermo SCIENTIFIC
Nitric Oxide (NO)	46.77	PPM	Model :	146i
Methane (CH ₄)	-	PPM	Serial Number :	1180540071
Carbon Monoxide (CO)	965.9			
Cylinder No. :	EB01159156			
Expiration Date :	Nov 06, 2026			

Multi-point gas test data

Reference Value (ppb)	Analyzer Display (ppb)	Difference Error	Percent Error	[% Error]
Level 1 Zero	0.0	0.00	0.00	0.00
Level 2 20.00%	100.0	100.7	0.70	0.70
Level 3 40.00%	200.0	200.6	0.30	0.30
Level 4 60.00%	300.0	300.7	0.23	0.23
Level 5 80.00%	400.0	400.0	0.00	0.00
Remark : Measuring Range	500.0 ppb	Average Difference (%)		0.25
:Acceptable Limit \pm 5%				

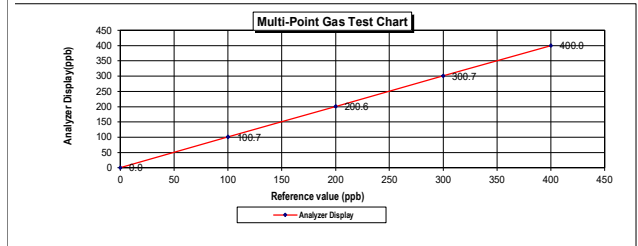

Calculate by : *[Signature]* Approve by : *[Signature]*
6 / 05 / 2025 6 / May / 2025

MULTI-POINT GAS TEST REPORT

Test Date : May 6, 2025


Equipment : Gas Analyzer (SO₂) Model : 43i
Manufacturer : Thermo SCIENTIFIC Serial Number : 1182920017

Standard Gas Concentration

Sulphur Dioxide (SO ₂)	42.89	PPM	Manufacturer :	Thermo SCIENTIFIC
Nitric Oxide (NO)	46.77	PPM	Model :	146i
Methane (CH ₄)	-	PPM	Serial Number :	1180540071
Carbon Monoxide (CO)	965.9			
Cylinder No. :	EB01159156			
Expiration Date :	Nov 06, 2026			

Multi-point gas test data

Reference Value (ppb)	Analyzer Display (ppb)	Difference Error	Percent Error	[% Error]
Level 1 Zero	0.0	0.00	0.00	0.00
Level 2 20.00%	100.0	100.6	0.60	0.60
Level 3 40.00%	200.0	200.7	0.35	0.35
Level 4 60.00%	300.0	301.0	0.33	0.33
Level 5 80.00%	400.0	400.0	0.00	0.00
Remark : Measuring Range	500.0 ppb	Average Difference (%)		0.26
:Acceptable Limit \pm 5%				

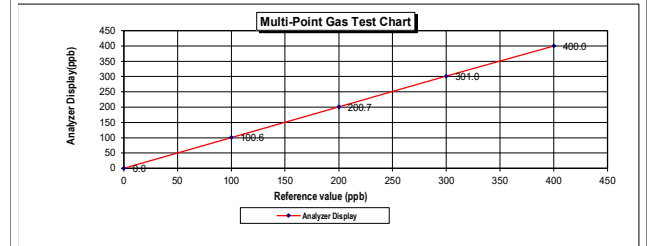

Calculate by : *[Signature]* Approve by : *[Signature]*
6 / 05 / 2025 6 / May / 2025

MULTI-POINT GAS TEST REPORT

Test Date : May 12, 2025


Equipment : Gas Analyzer (SO₂) Model : 43i
Manufacturer : Thermo SCIENTIFIC Serial Number : 1180540065

Standard Gas Concentration

Sulphur Dioxide (SO ₂)	42.89	PPM	Manufacturer :	Thermo SCIENTIFIC
Nitric Oxide (NO)	46.77	PPM	Model :	146i
Methane (CH ₄)	-	PPM	Serial Number :	1180540071
Carbon Monoxide (CO)	965.9			
Cylinder No. :	EB01159156			
Expiration Date :	Nov 06, 2026			

Multi-point gas test data

Reference Value (ppb)	Analyzer Display (ppb)	Difference Error	Percent Error	[% Error]
Level 1 Zero	0.0	0.00	0.00	0.00
Level 2 20.00%	100.0	100.7	0.70	0.70
Level 3 40.00%	200.0	200.7	0.35	0.35
Level 4 60.00%	300.0	300.5	0.17	0.17
Level 5 80.00%	400.0	400.0	0.00	0.00
Remark : Measuring Range	500.0 ppb	Average Difference (%)		0.24
:Acceptable Limit \pm 5%				

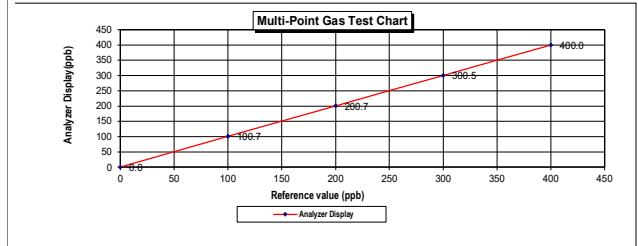

Calculate by : *[Signature]* Approve by : *[Signature]*
12 / 05 / 2025 12 / May / 2025

CERTIFICATE OF ANALYSIS

Grade of Product: EPA PROTOCOL STANDARD

Customer: AIR LIQUIDE (THAILAND)
LTD--
Part Number: E05N91E15A0014
Cylinder Number: EB0162121
Laboratory: 124 - Plumsteadville - PA
PGVP Number: A12023
Gas Code: CO, CO₂, NO, NO₂, SO₂, BALN

Reference Number: 160-402772205-1
Cylinder Volume: 144.0 CF
Cylinder Pressure: 2015 PSIG
Valve Outlet: 660
Certification Date: Jul 06, 2023
Expiration Date: Jul 06, 2031

Certification performed in accordance with EPA Traceability Protocol for Assay and Certification of Gaseous Calibration Standards (May 2012) document EPA 820-R-12-051, using the assay procedures listed. Analytical Methodology does not require correction for analytical interference. This cylinder has a total analytical uncertainty as stated below with a confidence level of 95%. There are no significant impurities which affect the use of this calibration mixture. All concentrations are on a mole/mole basis unless otherwise noted. The results relate only to the items tested. The report shall not be reproduced except in full without approval of the laboratory. Do Not Use This Cylinder below 100 psig, i.e. 3.7 megapascals.

ANALYTICAL RESULTS

Component	Requested Concentration	Actual Concentration	Protocol Method	Total Relative Uncertainty	Assay Dates
NOX	100.0 PPM	100.4 PPM	G1	\pm 0.9% NIST Traceable	06/27/2023, 07/06/2023
NITRIC OXIDE	100.0 PPM	100.2 PPM	G1	\pm 0.9% NIST Traceable	06/27/2023, 07/06/2023
SULFUR DIOXIDE	100.0 PPM	100.5 PPM	G1	\pm 1.4% NIST Traceable	06/27/2023, 07/06/2023
CARBON MONOXIDE	200.0 PPM	199.2 PPM	G1	\pm 0.3% NIST Traceable	06/26/2023
CARBON DIOXIDE	8,000 %	7,982 %	G1	\pm 1.3% NIST Traceable	06/27/2023
NITROGEN	Balance				

CALIBRATION STANDARDS

Type	Lot ID	Cylinder No	Concentration	Uncertainty	Expiration Date
GMIS	104202308	CG754364	98.36 PPM NITRIC OXIDE/NITROGEN	\pm 0.4%	Jan 04, 2031
PRM	C2219101	AP15154048	100.16 PPM NITRIC OXIDE/NITROGEN	\pm 0.3%	Feb 28, 2025
GMIS	2023042525	CG754361	98.62 PPM NITRIC OXIDE/NITROGEN	\pm 0.4%	Apr 25, 2031
PRM	12459	D913880	15.01 PPM NITROGEN DIOXIDE/AIR	\pm 1.5%	Feb 17, 2023
GMIS	153400202602	EB0130037	9.893 PPM NITROGEN DIOXIDE/NITROGEN	\pm 1.0%	Sep 29, 2025
NTRM	160102-22	KAL203620	97.69 PPM SULFUR DIOXIDE/NITROGEN	\pm 0.9%	Nov 01, 2027
CO	230801	CG745902	249.47 PPM CARBON MONOXIDE/NITROGEN	\pm 0.3%	Dec 09, 2028
NTRM	130606-02	CCA11730	13.359 % CARBON DIOXIDE/NITROGEN	\pm 0.5%	May 14, 2025

The SRM, NTRM, PRM, or RSM noted above is only in reference to the GMIS used in the assay and not part of the analysis.

ANALYTICAL EQUIPMENT

Instrument/Make/Model	Analytical Principle	Last Multipoint Calibration
Nicolet iS65 FTIR AUP2010245 CO2	FTIR	Jun 15, 2023
SIEMENS ULTRAMATE6E N1-CR-180	NDIR	Jun 14, 2023
Nicolet iS55 FTIR AUP2010245 NO	FTIR	Jun 29, 2023
Nicolet iS55 FTIR AUP2010245 NO2	FTIR	Jun 15, 2023
Nicolet iS55 FTIR AUP2010245 SO2	FTIR	Jun 08, 2023

[Signature]
Approved for Release

THAI METEOROLOGICAL DEPARTMENT



4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804,0-2399-0469

Calibration Certificate

Issued by : Calibration & Test Section : Meteorological Instruments Bureau

Date of Issue : 14 April, 2025

Certification No. : 215/25

Page : 1 of 2

Object : Weather Station

Manufacturer : Met One Instruments

Mode No. : Data Logger 466A Wind Sensor 034B

Mfg Code : Data Logger X4726 Wind Sensor N3282

Customer : United Analyst and Engineering Consultant Co.,Ltd.

81 Soi Udomsuk 41, Sukhumvit Road,
Bangchak, Prakanong, Bangkok 10260.

Calibration Condition : Temperature 25.1 °C Barometric Pressure 1013.2 hPa

NATIONAL STANDARD WIND TUNNEL : Thermal Anemometer 642 S/N 91563

: HOOK GAGE NO 1425 : Wind Aloft Plotting Board

N.I.S.T. Test Reference Number 731/241460

: Ultrasonic Anemometer Model DA-650-3TV (sensor TR-90AH)
Serial Number 110730029 (sensor 120629586)

JAPAN QUALITY ASSURANCE ORGANIZATION

Calibrated by :
Mr. Watchanop Subwat
Mechanical EngineerSigned :
Mr. Pisood Piamsut

(Authorized Signatory)

เอกสารไม่ควบคุม
Sub-Standard InstrumentINNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
71/9 MOO 13, SOI SUTHAPOKORN 11 TAMBON BANG KAE
AMPHOE BANG PHUEN SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL : 0640-2110-7600-1 FAX: 0640-2110-7140

Page 1 of 2.

Certificate of Calibration

Customer

Name : UNITED ANALYST AND ENGINEERING

Certificate No : 25-ACT-074

CONSULTANT CO.,LTD.

Request No : Req-2025-1018

Address : 81 Soi Udomsuk 41, Sukhumvit Road, Bangchak,
Prakanong, Bangkok 10260

Unit Under Calibration Details

Measurement item : Acoustic Calibrator

Class : 1

Manufacturer : LARSON DAVIS

Range : 94, 114 dB / 1000 Hz

Model : CAL200

Instrument Status : Used

Serial Number : 21091

ID : UAE.EFM.047/2566

Calibration Environment and Details

Temperature : (23 ±2 °C)

Humidity : (50 ± 20 %RH)

Barometric Pressure : (1013 ±10.0 hPa)

Received Date : 9 May 2025

Calibration Date : 20 May 2025

Location of Calibration : LAB 1 Acoustic

Calibration Procedure : In-house method CP-ACT-02 based on IEC 60942:2017 Electroacoustics - Sound calibrators

Reference Standard	Model	Serial Number	Traceable	Due Calibration
Sound Calibrator	SV 35A	58079	EEL	12 June 2025
THD Multimeter	2015	1047765	NIMT	4 February 2026

Traceability : This certificate provides traceability of measurement to recognized national standard, and to the realization of the international system of units (SI).

Note

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor $k=2$, providing a level of confidence approximately 95 %.Calibrated By :
Mr. Noppaden Luangart
Service Calibration EngineerApproved By :
Mr. Pacit Mathavorn
Calibration Engineer Supervisor

Issue Date : 20 May 2025

เอกสารไม่ควบคุม

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.
FM-708-ACT-02 Rev.04 Issue date 12/2/25

THAI METEOROLOGICAL DEPARTMENT



4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804,0-2399-0469

The Result of Calibration

Certification No. 215/25

14 April, 2025

Page : 2 of 2

Standard	HOOK GAGE NO. 1425			TESTED ANEMOMETER	
	Pressure	Vacuum	Pressure	Velocity	Correction
m/sec	inches	inches	hPa	m/sec	m/sec
1.00	-	-	-	1.00	0.00
3.02	-	-	-	3.03	-0.01
5.00	-	-	-	5.05	-0.05
7.00	-	-	-	7.09	-0.09
9.02	-	-	-	9.11	-0.09
11.01	-	-	-	11.13	-0.12
13.01	-	-	-	13.16	-0.15
15.01	-	-	-	15.20	-0.19
17.02	-	-	-	17.14	-0.12
20.02	-	-	-	20.16	-0.14

Wind Aloft Plotting Board.	
US DEPARTMENT OF COMMERCE WEATHER BUREAU	
WIND DIRECTION	TESTED WIND DIRECTION
0	0
90	91.2
180	181.1
270	270.2

Calibrated by :
Mr. Watchanop Subwat
Mechanical Engineer

Calibration & Test Section

Meteorological Instruments Bureau
เอกสารไม่ควบคุมINNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
71/9 MOO 13, SOI SUTHAPOKORN 11 TAMBON BANG KAE
AMPHOE BANG PHUEN SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL : 0640-2110-7600-1 FAX: 0640-2110-7140

Page 2 of 2.

Certificate No : 25-ACT-074

Request No : Req-2025-1018

Sound pressure level

Calibration Results : Without Adjustment

Calibration Range	Without Adjustment (dB)		Adjustment (dB)		Uncertainty
	Measured	Deviated value	Measured	Deviated value	(± dB)
94 dB / 1000 Hz	93.90	-0.10	-	-	0.11
114 dB / 1000 Hz	113.88	-0.14	-	-	0.11

Frequency of Sound pressure level

Calibration Range	Without Adjustment		Adjustment		Uncertainty
	Measured (Hz)	Deviated value	Measured (Hz)	Deviated value	(± %)
94 dB / 1000 Hz	1000.0	0.00	-	-	0.01
114 dB / 1000 Hz	1000.0	0.00	-	-	0.010

Total Harmonic Distortion plus Noise of Sound pressure level (THD+N %)

Calibration Range	Without Adjustment		Adjustment		Uncertainty
	Measured (%)		Measured (%)		(± %)
94 dB / 1000 Hz	1.89		-	-	0.17
114 dB / 1000 Hz	0.55		-	-	0.17

Note :

- The calibration results exclude the calibration pressure correction

- The calibration results exclude the microphone volume correction

End of Calibration

เอกสารไม่ควบคุม

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.
FM-708-ACT-02 Rev.04 Issue date 12/2/25



ELECTRICAL AND ELECTRONICS INSTITUTE FOUNDATION FOR INDUSTRIAL DEVELOPMENT

975 Moo 4, Bangpoo Industrial Estate, Soi 8, Sukhumvit Road km 37,
Phraek Sa, Mueang Samut Prakan, Samut Prakan 10280

Tel: +66 2709 4860 Fax: +66 2324 0917



NAC-MRA
NAC-MRA
NAC-MRA

Certificate No.: CP20240324EA
Operation No.: CP2024080295

Certificate of Calibration

Equipment: Sound Level Meter

Manufacturer: Larson Davis (Meter), PCB (Microphone), PCB (Preamplifier)

Model/Type: LxT1 (Meter), 377B02 (Microphone), PRMLxT1 (Preamplifier)

Serial No.: 0007302 (Meter), 344896 (Microphone), 0776637 (Preamplifier)

ID No.: UAE.EFM.035/2566

Customer: United Analyst and Engineering Consultant Co.,Ltd.

Address: 81 Soi Udomsuk 41, Sukhumvit Road, Bangchak
Phrakhanong, Bangkok 10260

Received Date: 9 August 2024

Calibrated Date: 22 - 27 August 2024

Issued Date: 28 August 2024

Calibrated by: Ms. Juntaporn Kunhakom

Approved by: 
(Mr. Sittichai Swaksuriyawong)
Group Manager

This report was prepared electronically using applicable electronic signature. Printing or copy of file are considered as a copy of the document.

The reported uncertainty of measurement was based on standard uncertainty multiplied by a coverage factor (k)
providing a level of confidence of approximately 95%. This certificate may not be reproduced other than in full except
with the prior written approval of the Electrical and Electronics Institute, Foundation for Industrial Development.

Page 1 of 6

เอกสารไม่ควบคุม

F-CAL-004 Ed.1



ELECTRICAL AND ELECTRONICS INSTITUTE FOUNDATION FOR INDUSTRIAL DEVELOPMENT

Certificate No.: CP20240324EA

Calibration Report

Equipment: Sound Level Meter

Manufacturer: Larson Davis (Meter), PCB (Microphone), PCB (Preamplifier)

Model/Type: LxT1 (Meter), 377B02 (Microphone), PRMLxT1 (Preamplifier)

Serial No.: 0007302 (Meter), 344896 (Microphone), 0776637 (Preamplifier)

ID No.: UAE.EFM.035/2566

Ambient Temperature: (23 ± 2) °C

Relative Humidity: (50 ± 15) %

Pressure: (101.3 ± 1.5) kPa

Method of Calibration :-
IEC 61672-3:2013.

Condition of this result of calibration

1. Reference standards instrument :-

Instrument	Model	Serial No.	Cert. No.	Due Date
1) Standard microphone	4180	2787490	AA-1012-23	12 November 2024
2) Arbitrary Function Generator	AFG2021	C010063	CK20240048EA	23 June 2025
3) Programmable Attenuator	PA5	2755	EF-0040-23	1 October 2024
4) 6.5 Digit precision multimeter	8846A	9610014	CB20230200EA	15 November 2024
5) Pressure humidity and Temperature Transmitter	PTU301	L3950483	CL1-P240023 CD20240142EA	24 March 2025 12 June 2025
6) Pressure humidity and Temperature Transmitter	PTU301	L3950484	CL1-P240030 CD20240143EA	11 April 2025 12 June 2025
7) Performance Audio Analyzer	U8903B	MY56510003	CB20240035EB CK20230072EA	13 February 2025 13 September 2024

2. This result of calibration was found accurate as shown on date and place of calibration only.

3. This certification is traceable to the international system of unit maintained at :-

Reference standards instrument for Acoustic function

- National Institute of Metrology (Thailand)

Reference standards instrument for Electrical function

- National Institute of Metrology (Thailand)

- Electrical and Electronics Institute; NSC Accredited Calibration No.0119

Result of Calibration:-

Function : 1. Indication at the calibration check frequency

Reference Acoustic Signal (dB)	Measured value (dB)	Deviation (dB)	Acceptance limits (dB)
-	-	-	-

Page 2 of 6

F-CAL-005 Ed.1

เอกสารไม่ควบคุม



ELECTRICAL AND ELECTRONICS INSTITUTE FOUNDATION FOR INDUSTRIAL DEVELOPMENT

Certificate No.: CP20240324EA

Calibration Report

Function : 2. Self-generated Noise

2.1 Microphone Installed

Measured value (dB)
28.8

2.2 Microphone replaced by the electrical input signal device

Frequency Weighting	Measured value (dB)
A-weighting	28.6
C-weighting	28.4
Z-weighting	34.3

Function : 3. Acoustical signal tests of frequency weightings (Without Windscreen)

Meter free-field acoustic response at a level of 84 dB.

Frequency (Hz)	Deviation from various Frequency Weighting Response Curve			
	C-Weighting (dB)	A-Weighting (dB)	Z-Weighting (dB)	Acceptance limits (dB)
125	0.1	0.1	0.1	±1.0
1000	0.0	0.0	0.0	±0.7
8000	-0.2	-0.2	-0.1	+1.5; -2.5

Function : 4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various Frequency Weighting Response Curve			
	C-Weighting (dB)	A-Weighting (dB)	Z-Weighting (dB)	Acceptance limits (dB)
63	-0.1	0.0	0.0	±1.0
125	0.0	0.0	-0.1	±1.0
250	-0.1	0.0	-0.1	±1.0
500	0.0	0.0	-0.1	±1.0
1000	0.0	0.0	0.0	±0.7
2000	0.0	0.0	0.0	±1.0
4000	0.0	0.0	0.0	±1.0
8000	-0.1	0.0	0.0	+1.5; -2.5
16000	0.0	0.0	-0.1	+2.5; -16.0

เอกสารไม่ควบคุม

Page 3 of 6

F-CAL-005 Ed.1



ELECTRICAL AND ELECTRONICS INSTITUTE FOUNDATION FOR INDUSTRIAL DEVELOPMENT

Certificate No.: CP20240324EA

Calibration Report

Function : 5. Frequency and time weighting at 1 kHz

5.1 Frequency weighting at 1 kHz

Frequency Weighting	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
C-weighting	94.0	0.0	±0.2
A-weighting	94.0	0.0	±0.2
Z-weighting	94.0	0.0	±0.2

5.2 Time weighting at 1 kHz

Time Weighting	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
Fast	94.0	0.0	±0.1
Slow	94.0	0.0	±0.1
LAeq	94.0	0.0	±0.1

Function : 6. Long-Term Stability

Long-term stability over 30 minutes, with steady 1 kHz signal at reference level.

Time Period to Apply Signal (min)	Reference SPL (dB)	Record SPL at Conclusion of Time Period (dB)	Deviated value (dB)	Acceptance limits (dB)
30	94.0	94.0	0.0	±0.1

Function : 7. Level Linearity on the reference level range

7.1 Level Linearity on the reference level range, Upper

Anticipated Value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
94.0	94.0	0.0	±0.8
99.0	99.0	0.0	±0.8
104.0	104.0	0.0	±0.8
109.0	109.0	0.0	±0.8
114.0	114.0	0.0	±0.8
119.0	119.0	0.0	±0.8
124.0	124.0	0.0	±0.8
129.0	129.0	0.0	±0.8
134.0	134.0	0.0	±0.8
139.0	139.0	0.0	±0.8

เอกสารไม่ควบคุม

Page 4 of 6

F-CAL-005 Ed.1

Certificate No.: CP20240324EA

Calibration Report

7.2 Level Linearity on the reference level range, Lower

Anticipated Value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
94.0	94.0	0.0	±0.8
89.0	89.0	0.0	±0.8
84.0	84.0	0.0	±0.8
79.0	79.0	0.0	±0.8
74.0	74.0	0.0	±0.8
69.0	69.0	0.0	±0.8
64.0	64.0	0.0	±0.8
59.0	59.0	0.0	±0.8
54.0	54.0	0.0	±0.8
49.0	49.0	0.0	±0.8
44.0	44.1	0.1	±0.8
39.0	39.4	0.4	±0.8

Function : 8. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
Fast	200	136.0	0.0	±0.5
	2	118.8	-0.2	+1.0 ; -1.5
	0.25	109.7	-0.3	+1.0 ; -3.0
Slow	200	129.5	-0.1	±0.5
	2	109.9	-0.1	+1.0 ; -3.0
	200	130.0	0.0	±0.5
LAE	2	110.0	0.0	+1.0 ; -1.5
	0.25	100.9	-0.1	+1.0 ; -3.0

Function : 9. Peak C sound level

Number of cycles in test signal	Anticipated Value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
Complete cycle	135.4	134.8	-0.6	±2.0
Positive half cycle	134.4	134.0	-0.4	±1.0
Negative half cycle	134.4	134.1	-0.3	±1.0

Page 5 of 6

F-CAL-005 Ed.1

เอกสารไม่ควบคุม

Certificate No.: CP20240324EA

Calibration Report

Function : 10. Overload indication

Measured value (dB)		Deviated value (dB)	Acceptance limits (dB)
Positive one-half cycle	Negative one-half cycle		
143.6	143.4	-0.2	±1.5

Function : 11. High-Level Stability

High-level stability over 5 minutes, with steady 1 kHz signal, 1 dB below upper boundary.

Time Period to Apply Signal (min)	Reference SPL (dB)	Record SPL at Conclusion of Time Period (dB)	Deviated value (dB)	Acceptance limits (dB)
5	139.0	139.0	0.0	±0.1

Uncertainty of measurement

Function	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1) Indication at the calibration check frequency	0.30	Not applicable
2) Self-generated Noise	0.10	Not applicable
3) Acoustical signal tests of frequency weightings - Free-field sound pressure response level	0.30	0.60 (10Hz to 4kHz) 0.70 (>4kHz to 10kHz)
4) Electrical signal tests of frequency weightings	0.20	0.20
5) Frequency and time weighting at 1 kHz	0.20	0.20
6) Long-Term Stability	0.10	0.10
7) Level Linearity on the reference level range	0.30	0.30
8) Tone burst response	0.20	0.30
9) Peak C sound level	0.20	0.35
10) Overload indication	0.20	0.25
11) High-Level Stability	0.10	0.10

Remarks:

1. Indication at the calibration check frequency can not measured because customer does not provide a sound calibrator.
2. The acceptance limit is for the deviated value.
3. Acceptance limits was IEC61672-3:2013 Class 1.
4. The coverage factor $k = 2.00$

- - End of Report - -

Page 6 of 6

F-CAL-005 Ed.1

เอกสารไม่ควบคุม



ELECTRICAL AND ELECTRONICS INSTITUTE
FOUNDATION FOR INDUSTRIAL DEVELOPMENT
975 Moo 4, Bangpoo Industrial Estate, Soi 8, Sukhumvit Road km 37,
Phraek Sa, Muang Samut Prakan, Samut Prakan 10280
Tel: +66 2709 4860 Fax: +66 2324 0917



ISO 15189:2013
CALIBRATION BODY

Certificate No.: CP20240339EA
Operation No.: CP2024090310

Certificate of Calibration

Equipment: Sound Level Meter
Manufacturer: Larson Davis (Meter), PCB (Microphone), PCB (Preamplifier)
Model/Type: LxT1 (Meter), 377B02 (Microphone), PRMLxT1 (Preamplifier)
Serial No.: 0007303 (Meter), 345232 (Microphone), 077638 (Preamplifier)
ID No.: UAE.EFM.036/2566
Customer: United Analyst and Engineering Consultant Co.,Ltd.
Address: 81 Soi Udomsuk 41, Sukhumvit Road, Bangchak Phrakhanong, Bangkok 10260
Received Date: 3 September 2024
Calibrated Date: 20 - 24 September 2024
Issued Date: 26 September 2024
Calibrated by: Ms. Juntaporn Kunhakom
Approved by: 
(Mr. Sittichai Swaksurlyawong)
Group Manager
This report was prepared electronically using applicable electronic signature. Printing or copy of file are considered as a copy of the document.
The reported uncertainty of measurement was based on standard uncertainty multiplied by a coverage factor (k) providing a level of confidence of approximately 95%. This certificate may not be reproduced other than in full except with the prior written approval of the Electrical and Electronics Institute, Foundation for Industrial Development.

Page 1 of 6

F-CAL-004 Ed.1

เอกสารไม่ควบคุม

Certificate No.: CP20240339EA

Calibration Report

Equipment: Sound Level Meter
Manufacturer: Larson Davis (Meter), PCB (Microphone), PCB (Preamplifier)
Model/Type: LxT1 (Meter), 377B02 (Microphone), PRMLxT1 (Preamplifier)
Serial No.: 0007303 (Meter), 345232 (Microphone), 077638 (Preamplifier)
ID No.: UAE.EFM.036/2566
Ambient Temperature: (23 ± 2) °C
Relative Humidity: (50 ± 15) %
Pressure: (101.3 ± 1.5) kPa
Method of Calibration :-
IEC 61672-3:2013.
Condition of this result of calibration
1. Reference standards instrument :-

Instrument	Model	Serial No.	Cert. No.	Due Date
1) Standard microphone	4180	2787490	AA-1012-23	12 November 2024
2) Arbitrary Function Generator	AFG2021	C010063	CK20240048EA	23 June 2025
3) Programmable Attenuator	PAS	2755	EF-0040-23	1 October 2024
4) 6.5 Digit precision multimeter	8846A	9610014	CB20230200EA	15 November 2024
5) Pressure humidity and Temperature Transmitter	PTU301	F0640002	CL1-P240022 CD20240180EA	20 March 2025 7 August 2025
6) Performance Audio Analyzer	U8903B	MY56510003	CB202400355EB CK20240069EA	13 February 2025 19 September 2025

2. This result of calibration was found accurate as shown on date and place of calibration only.
3. This certification is traceable to the international system of unit maintained at :-
Reference standards instrument for Acoustic function
- National Institute of Metrology (Thailand)
- Electrical and Electronics Institute; NSC Accredited Calibration No.0119
Reference standards instrument for Electrical function
- National Institute of Metrology (Thailand)
- Electrical and Electronics Institute; NSC Accredited Calibration No.0119

Result of Calibration:-

Function : 1. Indication at the calibration check frequency

Reference Acoustic Signal (dB)	Measured value (dB)	Deviation (dB)	Acceptance limits (dB)
-	-	-	-

Page 2 of 6

F-CAL-005 Ed.1

เอกสารไม่ควบคุม

Certificate No.: CP20240339EA

Calibration Report

Function : 2. Self-generated Noise
2.1 Microphone Installed

Measured value (dB)
29.7

2.2 Microphone replaced by the electrical input signal device

Frequency Weighting	Measured value (dB)
A-weighting	29.6
C-weighting	29.5
Z-weighting	35.1

Function : 3. Acoustical signal tests of frequency weightings (Without Windscreen)
Meter free-field acoustic response at a level of 84 dB.

Frequency (Hz)	Deviation from various Frequency Weighting Response Curve			
	C-Weighting (dB)	A-Weighting (dB)	Z-Weighting (dB)	Acceptance limits (dB)
125	0.5	0.4	0.4	±1.0
1000	-0.1	-0.1	-0.1	±0.7
8000	0.3	0.3	0.3	+1.5; -2.5

Function : 4. Electrical signal tests of frequency weightings
Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various Frequency Weighting Response Curve			
	C-Weighting (dB)	A-Weighting (dB)	Z-Weighting (dB)	Acceptance limits (dB)
63	0.0	0.0	0.0	±1.0
125	0.0	0.0	0.0	±1.0
250	0.0	0.0	0.0	±1.0
500	0.1	-0.1	0.0	±1.0
1000	0.0	0.0	0.0	±0.7
2000	0.0	0.0	0.1	±1.0
4000	0.0	0.0	0.0	±1.0
8000	-0.1	-0.1	0.1	+1.5; -2.5
16000	0.0	0.0	0.0	+2.5; -16.0

Certificate No.: CP20240339EA

Calibration Report

Function : 5. Frequency and time weighting at 1 kHz
5.1 Frequency weighting at 1 kHz

Frequency Weighting	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
C-weighting	94.0	0.0	±0.2
A-weighting	94.0	0.0	±0.2
Z-weighting	94.0	0.0	±0.2

5.2 Time weighting at 1 kHz

Time Weighting	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
Fast	94.0	0.0	±0.1
Slow	94.0	0.0	±0.1
LReq	94.0	0.0	±0.1

Function : 6. Long-Term Stability

Long-term stability over 30 minutes, with steady 1 kHz signal at reference level.

Time Period to Apply Signal (min)	Reference SPL (dB)	Record SPL at Conclusion of Time Period (dB)	Deviated value (dB)	Acceptance limits (dB)
30	94.0	94.0	0.0	±0.1

Function : 7. Level Linearity on the reference level range
7.1 Level Linearity on the reference level range, Upper

Anticipated Value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
94.0	94.0	0.0	±0.8
99.0	99.0	0.0	±0.8
104.0	104.0	0.0	±0.8
109.0	109.0	0.0	±0.8
114.0	114.0	0.0	±0.8
119.0	119.0	0.0	±0.8
124.0	124.0	0.0	±0.8
129.0	129.0	0.0	±0.8
134.0	134.1	0.1	±0.8
139.0	139.1	0.1	±0.8
140.0	140.1	0.1	±0.8

Certificate No.: CP20240339EA

Calibration Report

7.2 Level Linearity on the reference level range, Lower

Anticipated Value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
94.0	94.0	0.0	±0.8
89.0	89.0	0.0	±0.8
84.0	84.0	0.0	±0.8
79.0	79.0	0.0	±0.8
74.0	74.0	0.0	±0.8
69.0	69.0	0.0	±0.8
64.0	64.0	0.0	±0.8
59.0	59.0	0.0	±0.8
54.0	54.0	0.0	±0.8
49.0	49.0	0.0	±0.8
44.0	44.1	0.1	±0.8
43.0	43.1	0.1	±0.8
42.0	42.2	0.2	±0.8
41.0	41.3	0.3	±0.8
40.0	40.4	0.4	±0.8

Function : 8. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
Fast	200	135.9	-0.1	±0.5
	2	118.8	-0.2	+1.0; -1.5
	0.25	109.8	-0.2	+1.0; -3.0
Slow	200	129.5	-0.1	±0.5
	2	109.9	-0.1	+1.0; -3.0
	0.25	110.0	0.0	±0.5
LAE	200	130.0	0.0	+1.0; -1.5
	0.25	101.0	0.0	+1.0; -3.0

Function : 9. Peak C sound level

Number of cycles in test signal	Anticipated Value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
Complete cycle	135.4	134.8	-0.6	±2.0
Positive half cycle	134.4	134.0	-0.4	±1.0
Negative half cycle	134.4	134.0	-0.4	±1.0

Certificate No.: CP20240339EA

Calibration Report

Function : 10. Overload Indication

Measured value (dB)		Deviated value (dB)	Acceptance limits (dB)
Positive one-half cycle	Negative one-half cycle		
143.6	143.5	-0.1	±1.5

Function : 11. High-Level Stability

High-level stability over 5 minutes, with steady 1 kHz signal, 1 dB below upper boundary.

Time Period to Apply Signal (min)	Reference SPL (dB)	Record SPL at Conclusion of Time Period (dB)	Deviated value (dB)	Acceptance limits (dB)
5	139.0	139.0	0.0	±0.1

Uncertainty of measurement

Function	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1) Indication at the calibration check frequency	0.30	Not applicable
2) Self-generated Noise	0.10	Not applicable
3) Acoustical signal tests of frequency weightings - Free-field sound pressure response level	0.30	0.60 (10Hz to 4kHz) 0.70 (>4kHz to 10kHz)
4) Electrical signal tests of frequency weightings	0.20	0.20
5) Frequency and time weighting at 1 kHz	0.20	0.20
6) Long-Term Stability	0.10	0.10
7) Level Linearity on the reference level range	0.30	0.30
8) Tone burst response	0.20	0.30
9) Peak C sound level	0.20	0.35
10) Overload indication	0.24	0.25
11) High-Level Stability	0.10	0.10

- Remarks:
1. Indication at the calibration check frequency can not measured because customer does not provide a sound calibrator.
 2. The acceptance limit is for the deviated value.
 3. Acceptance limits was IEC61672-3:2013 Class 1.
 4. The coverage factor $k = 2.00$

-- End of Report --



Certificate No.: CP20240340EA
Operation No.: CP2024090311

Certificate of Calibration

Equipment: Sound Level Meter
Manufacturer: Larson Davis (Meter), PCB (Microphone), PCB (Preamplifier)
Model/Type: LxT1 (Meter), 377B02 (Microphone), PRMLxT1 (Preamplifier)
Serial No.: 0007304 (Meter), 345233 (Microphone), 077639 (Preamplifier)
ID No.: UAE.EFM.037/2566
Customer: United Analyst and Engineering Consultant Co., Ltd.
Address: 81 Soi Udomsuk 41, Sukhumvit Road, Bangchak Phrakhanong, Bangkok 10260
Received Date: 3 September 2024
Calibrated Date: 20 - 24 September 2024
Issued Date: 26 September 2024
Calibrated by: Ms. Juntaporn Kunhakom

Approved by:

(Mr. Sittichai Swaksuriyawong)
Group Manager

This report was prepared electronically using applicable electronic signature. Printing or copy of file are considered as a copy of this document.
The reported uncertainty of measurement was based on standard uncertainty multiplied by a coverage factor (k) providing a level of confidence of approximately 95%. This certificate may not be reproduced other than in full except with the prior written approval of the Electrical and Electronics Institute, Foundation for Industrial Development.

Page 1 of 6

F-CAL-004 Ed.1

เอกสารไม่ควบคุม



Certificate No.: CP20240340EA

Calibration Report

Equipment: Sound Level Meter
Manufacturer: Larson Davis (Meter), PCB (Microphone), PCB (Preamplifier)
Model/Type: LxT1 (Meter), 377B02 (Microphone), PRMLxT1 (Preamplifier)
Serial No.: 0007304 (Meter), 345233 (Microphone), 077639 (Preamplifier)
ID No.: UAE.EFM.037/2566
Ambient Temperature: (23 ± 2) °C
Relative Humidity: (50 ± 15) %
Pressure: (101.3 ± 1.5) kPa
Method of Calibration :-
IEC 61672-3:2013.
Condition of this result of calibration
1. Reference standards instrument :-

Instrument	Model	Serial No.	Cert. No.	Due Date
1) Standard microphone	4180	2787490	AA-1012-23	12 November 2024
2) Arbitrary Function Generator	AFG2021	CD10063	CK20240048EA	23 June 2025
3) Programmable Attenuator	PA5	2755	EF-0040-23	1 October 2024
4) 6.5 Digit precision multimeter	8846A	9610014	CB20230200EA	15 November 2024
5) Pressure humidity and Temperature Transmitter	PTU301	F0640002	CL1-P240022 CD20240180EA	20 March 2025 7 August 2025
6) Performance Audio Analyzer	U8903B	MY5610003	CB20240035EB CK20240069EA	13 February 2025 19 September 2025

2. This result of calibration was found accurate as shown on date and place of calibration only.

3. This certification is traceable to the international system of unit maintained at :-

Reference standards instrument for Acoustic function

- National Institute of Metrology (Thailand)

- Electrical and Electronics Institute; NSC Accredited Calibration No.0119

Reference standards instrument for Electrical function

- National Institute of Metrology (Thailand)

- Electrical and Electronics Institute; NSC Accredited Calibration No.0119

Result of Calibration:-

Function : 1. Indication at the calibration check frequency

Reference Acoustic Signal (dB)	Measured value (dB)	Deviation (dB)	Acceptance limits (dB)
-	-	-	-

Page 2 of 6

F-CAL-005 Ed.1

เอกสารไม่ควบคุม



Certificate No.: CP20240340EA

Calibration Report

Function : 2. Self-generated Noise

2.1 Microphone Installed

Measured value (dB)
28.5

2.2 Microphone replaced by the electrical input signal device

Frequency Weighting	Measured value (dB)
A-weighting	28.4
C-weighting	28.2
Z-weighting	34.4

Function : 3. Acoustical signal tests of frequency weightings (Without Windscreens)

Meter free-field acoustic response at a level of 84 dB.

Frequency (Hz)	Deviation from various Frequency Weighting Response Curve			
	C-Weighting (dB)	A-Weighting (dB)	Z-Weighting (dB)	Acceptance limits (dB)
125	0.2	0.0	0.1	±1.0
1000	0.0	0.0	0.0	±0.7
8000	-0.4	-0.4	-0.3	+1.5, -2.5

Function : 4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various Frequency Weighting Response Curve			
	C-Weighting (dB)	A-Weighting (dB)	Z-Weighting (dB)	Acceptance limits (dB)
63	0.0	0.1	0.0	±1.0
125	0.0	0.0	-0.1	±1.0
250	0.0	0.0	-0.1	±1.0
500	0.0	0.0	0.0	±1.0
1000	0.0	0.0	0.0	±0.7
2000	0.0	0.0	0.0	±1.0
4000	0.0	0.0	0.0	±1.0
8000	-0.1	0.0	0.0	+1.5, -2.5
16000	0.0	0.1	-0.1	+2.5, -16.0

Page 3 of 6

F-CAL-005 Ed.1

เอกสารไม่ควบคุม



Certificate No.: CP20240340EA

Calibration Report

Function : 5. Frequency and time weighting at 1 kHz

5.1 Frequency weighting at 1 kHz

Frequency Weighting	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
C-weighting	94.0	0.0	±0.2
A-weighting	94.0	0.0	±0.2
Z-weighting	94.0	0.0	±0.2

5.2 Time weighting at 1 kHz

Time Weighting	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
Fast	94.0	0.0	±0.1
Slow	94.0	0.0	±0.1
LAeq	94.0	0.0	±0.1

Function : 6. Long-Term Stability

Long-term stability over 30 minutes, with steady 1 kHz signal at reference level.

Time Period to Apply Signal (min)	Reference SPL (dB)	Record SPL at Conclusion of Time Period (dB)	Deviated value (dB)	Acceptance limits (dB)
30	94.0	94.0	0.0	±0.1

Function : 7. Level Linearity on the reference level range

7.1 Level Linearity on the reference level range, Upper

Anticipated Value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
94.0	94.0	0.0	±0.8
99.0	99.0	0.0	±0.8
104.0	104.0	0.0	±0.8
109.0	109.0	0.0	±0.8
114.0	114.0	0.0	±0.8
119.0	119.0	0.0	±0.8
124.0	124.0	0.0	±0.8
129.0	129.0	0.0	±0.8
134.0	134.1	0.1	±0.8
139.0	139.1	0.1	±0.8

Page 4 of 6

F-CAL-005 Ed.1

เอกสารไม่ควบคุม

Certificate No.: CP20240340EA

Calibration Report

7.2 Level Linearity on the reference level range, Lower

Anticipated Value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
94.0	94.0	0.0	±0.8
89.0	89.0	0.0	±0.8
84.0	84.0	0.0	±0.8
79.0	79.0	0.0	±0.8
74.0	74.0	0.0	±0.8
69.0	69.0	0.0	±0.8
64.0	64.0	0.0	±0.8
59.0	59.0	0.0	±0.8
54.0	54.0	0.0	±0.8
49.0	49.0	0.0	±0.8
44.0	44.1	0.1	±0.8
43.0	43.1	0.1	±0.8
42.0	42.1	0.1	±0.8
41.0	41.2	0.2	±0.8
40.0	40.3	0.3	±0.8
39.0	39.3	0.3	±0.8
38.0	38.4	0.4	±0.8
37.0	37.6	0.6	±0.8

Function : 8. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
Fast	200	135.9	-0.1	±0.5
	2	118.8	-0.2	+1.0 ; -1.5
	0.25	109.8	-0.2	+1.0 ; -3.0
Slow	200	129.5	-0.1	±0.5
	2	109.9	-0.1	+1.0 ; -3.0
	200	130.0	0.0	±0.5
LAE	2	109.9	-0.1	+1.0 ; -1.5
	0.25	101.0	0.0	+1.0 ; -3.0

Function : 9. Peak C sound level

Number of cycles in test signal	Anticipated Value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
Complete cycle	135.4	134.7	-0.7	±2.0
Positive half cycle	134.4	134.0	-0.4	±1.0
Negative half cycle	134.4	134.0	-0.4	±1.0

Page 5 of 6

F-CAL-005 Ed.1

เอกสารไม่ควบคุม

Certificate No.: CP20240340EA

Calibration Report

Function : 10. Overload Indication

Measured value (dB)		Deviated value (dB)	Acceptance limits (dB)
Positive one-half cycle	Negative one-half cycle		
142.6	142.5	-0.1	±1.5

Function : 11. High-Level Stability

High-level stability over 5 minutes, with steady 1 kHz signal, 1 dB below upper boundary.

Time Period to Apply Signal (min)	Reference SPL (dB)	Record SPL at Conclusion of Time Period (dB)	Deviated value (dB)	Acceptance limits (dB)
5	139.0	139.0	0.0	±0.1

Uncertainty of measurement

Function	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1) Indication at the calibration check frequency	0.30	Not applicable
2) Self-generated Noise	0.10	Not applicable
3) Acoustical signal tests of frequency weightings - Free-field sound pressure response level	0.30	0.60 (10Hz to 4kHz) 0.70 (>4kHz to 10kHz)
4) Electrical signal tests of frequency weightings	0.20	0.20
5) Frequency and time weighting at 1 kHz	0.20	0.20
6) Long-Term Stability	0.10	0.10
7) Level Linearity on the reference level range	0.30	0.30
8) Tone burst response	0.20	0.30
9) Peak C sound level	0.20	0.35
10) Overload indication	0.24	0.25
11) High-Level Stability	0.10	0.10

- Remarks:
- The acceptance limit is for the deviated value.
 - Acceptance limits was IEC61672-3:2013 Class 1.
 - The coverage factor $k = 2.00$

-- End of Report --

Page 6 of 6

F-CAL-005 Ed.1

เอกสารไม่ควบคุม

Certificate No.: CP20240323EA
Operation No.: CP2024080294

Certificate of Calibration

Equipment: Sound Level Meter

Manufacturer: Larson Davis (Meter), PCB (Microphone), PCB (Preamplifier)

Model/Type: LxT1 (Meter), 377B02 (Microphone), PRMLxT1 (Preamplifier)

Serial No.: 0007305 (Meter), 345234 (Microphone), 077640 (Preamplifier)

ID No.: UAE.EFM.038/2566

Customer: United Analyst and Engineering Consultant Co.,Ltd.

Address: 81 Soi Udomsuk 41, Sukhumvit Road, Bangchak Phraekhanong, Bangkok 10260

Received Date: 9 August 2024

Calibrated Date: 22 - 27 August 2024

Issued Date: 28 August 2024

Calibrated by: Ms. Juntaporn Kunhakom

Approved by:

(Mr. Sittichai Swaksuriyawong)
Group Manager

This report was prepared electronically using applicable electronic signature. Printing or copy of file are considered as a copy of the document.

The reported uncertainty of measurement was based on standard uncertainty multiplied by a coverage factor (k) providing a level of confidence of approximately 95%. This certificate may not be reproduced other than in full except with the prior written approval of the Electrical and Electronics Institute, Foundation for Industrial Development.

Page 1 of 6

เอกสารไม่ควบคุม

F-CAL-004 Ed.1

Certificate No.: CP20240323EA

Calibration Report

Equipment: Sound Level Meter

Manufacturer: Larson Davis (Meter), PCB (Microphone), PCB (Preamplifier)

Model/Type: LxT1 (Meter), 377B02 (Microphone), PRMLxT1 (Preamplifier)

Serial No.: 0007305 (Meter), 345234 (Microphone), 077640 (Preamplifier)

ID No.: UAE.EFM.038/2566

Ambient Temperature: (23 ± 2) °C

Relative Humidity: (50 ± 15) %

Pressure: (101.3 ± 1.5) kPa

Method of Calibration :- IEC 61672-3:2013.

Condition of this result of calibration

1. Reference standards instrument :-

Instrument	Model	Serial No.	Cert. No.	Due Date
1) Standard microphone	4180	2787490	AA-1012-23	12 November 2024
2) Arbitrary Function Generator	AFG2021	C010063	CK20240048EA	23 June 2025
3) Programmable Attenuator	PA5	2755	EF-0040-23	1 October 2024
4) 6.5 Digit precision multimeter	8846A	9610014	CB20230200EA	15 November 2024
5) Pressure humidity and Temperature Transmitter	PTU301	L3950483	CL1-P240023 CD20240142EA	24 March 2025 12 June 2025
6) Pressure humidity and Temperature Transmitter	PTU301	L3950484	CL1-P240030 CD20240143EA	11 April 2025 12 June 2025
7) Performance Audio Analyzer	U8903B	MY56510003	CB20240035EB CK20230072EA	13 February 2025 13 September 2024

2. This result of calibration was found accurate as shown on date and place of calibration only.

3. This certification is traceable to the international system of unit maintained at :-

- Reference standards instrument for Acoustic function
- National Institute of Metrology (Thailand)
- Reference standards instrument for Electrical function
- National Institute of Metrology (Thailand)
 - Electrical and Electronics Institute; NSC Accredited Calibration No.0119

Result of Calibration:-

Function : 1. Indication at the calibration check frequency

Reference Acoustic Signal (dB)	Measured value (dB)	Deviation (dB)	Acceptance limits (dB)
-	-	-	-

Page 2 of 6

F-CAL-005 Ed.1

เอกสารไม่ควบคุม

Certificate No.: CP20240323EA

Calibration Report

Function : 2. Self-generated Noise

2.1 Microphone Installed

Measured value (dB)
30.1

2.2 Microphone replaced by the electrical input signal device

Frequency Weighting (dB)	Measured value (dB)
A-weighting	29.9
C-weighting	30.0
Z-weighting	35.5

Function : 3. Acoustical signal tests of frequency weightings (Without Windscreen)

Meter free-field acoustic response at a level of 84 dB.

Frequency (Hz)	Deviation from various Frequency Weighting Response Curve			
	C-Weighting (dB)	A-Weighting (dB)	Z-Weighting (dB)	Acceptance limits (dB)
125	0.2	0.1	0.1	±1.0
1000	-0.1	-0.1	-0.1	±0.7
8000	0.6	0.5	0.6	+1.5; -2.5

Function : 4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various Frequency Weighting Response Curve			
	C-Weighting (dB)	A-Weighting (dB)	Z-Weighting (dB)	Acceptance limits (dB)
63	0.0	-0.1	0.0	±1.0
125	0.0	-0.1	0.0	±1.0
250	0.0	-0.1	0.0	±1.0
500	0.0	-0.1	0.0	±1.0
1000	0.0	0.0	0.0	±0.7
2000	0.0	-0.1	0.0	±1.0
4000	0.0	-0.1	0.0	±1.0
8000	-0.1	-0.1	0.0	+1.5; -2.5
16000	0.0	0.0	0.0	+2.5; -16.0

เอกสารไม่ควบคุม

Page 3 of 6

F-CAL-005 Ed.1

Certificate No.: CP20240323EA

Calibration Report

Function : 5. Frequency and time weighting at 1 kHz

5.1 Frequency weighting at 1 kHz

Frequency Weighting	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
C-weighting	94.0	0.0	±0.2
A-weighting	94.0	0.0	±0.2
Z-weighting	94.0	0.0	±0.2

5.2 Time weighting at 1 kHz

Time Weighting	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
Fast	94.0	0.0	±0.1
Slow	94.0	0.0	±0.1
LAeq	94.0	0.0	±0.1

Function : 6. Long-Term Stability

Long-term stability over 30 minutes, with steady 1 kHz signal at reference level.

Time Period to Apply Signal (min)	Reference SPL (dB)	Record SPL at Conclusion of Time Period (dB)	Deviated value (dB)	Acceptance limits (dB)
30	94.0	94.0	0.0	±0.1

Function : 7. Level Linearity on the reference level range

7.1 Level Linearity on the reference level range, Upper

Anticipated Value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
94.0	94.0	0.0	±0.8
99.0	99.0	0.0	±0.8
104.0	104.0	0.0	±0.8
109.0	109.0	0.0	±0.8
114.0	114.0	0.0	±0.8
119.0	119.0	0.0	±0.8
124.0	124.0	0.0	±0.8
129.0	129.0	0.0	±0.8
134.0	134.0	0.0	±0.8
139.0	139.0	0.0	±0.8
140.0	140.0	0.0	±0.8
141.0	141.0	0.0	±0.8

เอกสารไม่ควบคุม

Page 4 of 6

F-CAL-005 Ed.1

Certificate No.: CP20240323EA

Calibration Report

7.2 Level Linearity on the reference level range, Lower

Anticipated Value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
94.0	94.0	0.0	±0.8
89.0	89.0	0.0	±0.8
84.0	84.0	0.0	±0.8
79.0	79.0	0.0	±0.8
74.0	74.0	0.0	±0.8
69.0	69.0	0.0	±0.8
64.0	64.0	0.0	±0.8
59.0	59.0	0.0	±0.8
54.0	54.0	0.0	±0.8
49.0	49.0	0.0	±0.8
44.0	44.1	0.1	±0.8
39.0	39.4	0.4	±0.8

Function : 8. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
Fast	200	136.0	0.0	±0.5
	2	118.9	-0.1	+1.0 ; -1.5
	0.25	109.7	-0.3	+1.0 ; -3.0
Slow	200	129.5	-0.1	±0.5
	2	109.9	-0.1	+1.0 ; -3.0
	200	130.0	0.0	±0.5
LAE	2	110.0	0.0	+1.0 ; -1.5
	0.25	100.9	-0.1	+1.0 ; -3.0

Function : 9. Peak C sound level

Number of cycles in test signal	Anticipated Value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
Complete cycle	135.4	134.8	-0.6	±2.0
Positive half cycle	134.4	134.0	-0.4	±1.0
Negative half cycle	134.4	134.0	-0.4	±1.0

เอกสารไม่ควบคุม

Page 5 of 6

F-CAL-005 Ed.1

Certificate No.: CP20240323EA

Calibration Report

Function : 10. Overload indication

Measured value (dB)		Deviated value (dB)	Acceptance limits (dB)
Positive one-half cycle	Negative one-half cycle		
143.7	143.7	0.0	±1.5

Function : 11. High-Level Stability

High-level stability over 5 minutes, with steady 1 kHz signal, 1 dB below upper boundary.

Time Period to Apply Signal (min)	Reference SPL (dB)	Record SPL at Conclusion of Time Period (dB)	Deviated value (dB)	Acceptance limits (dB)
5	139.0	139.0	0.0	±0.1

Uncertainty of measurement

Function	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1) Indication at the calibration check frequency	0.30	Not applicable
2) Self-generated Noise	0.10	Not applicable
3) Acoustical signal tests of frequency weightings - Free-field sound pressure response level	0.30	0.60 (10Hz to 4kHz) 0.70 (>4kHz to 10kHz)
4) Electrical signal tests of frequency weightings	0.20	0.20
5) Frequency and time weighting at 1 kHz	0.20	0.20
6) Long-Term Stability	0.10	0.10
7) Level Linearity on the reference level range	0.30	0.30
8) Tone burst response	0.20	0.30
9) Peak C sound level	0.20	0.35
10) Overload indication	0.20	0.25
11) High-Level Stability	0.10	0.10

Remarks:

1. Indication at the calibration check frequency can not measured because customer does not provide a sound calibrator.
2. The acceptance limit is for the deviated value.
3. Acceptance limits was IEC61672-3:2013 Class 1.
4. The coverage factor $k = 2.00$

- - End of Report - -

เอกสารไม่ควบคุม

Page 6 of 6

F-CAL-005 Ed.1



ELECTRICAL AND ELECTRONICS INSTITUTE
FOUNDATION FOR INDUSTRIAL DEVELOPMENT

975 Moo 4, Bangpoo Industrial Estate, Soi 8, Sukhumvit Road km 37,
Phraek Sa, Mueang Samut Prakan, Samut Prakan 10280

Tel: +66 2709 4860 Fax: +66 2324 0917



Certificate No.: CP20240290EA
Operation No.: CP2024070253

Certificate of Calibration

Equipment: Sound Level Meter

Manufacturer: Larson Davis (Meter), PCB (Microphone), PCB (Preamplifier)

Model/Type: LxT1 (Meter), 377B02 (Microphone), PRMLxT1 (Preamplifier)

Serial No.: 0007306 (Meter), 345235 (Microphone), 077641 (Preamplifier)

ID No.: UAE.EFM.039/2566

Customer: United Analyst and Engineering Consultant Co.,Ltd.

Address: 81 Soi Udomsuk 41, Sukhumvit Road, Bangchak
Phrakhanong, Bangkok 10260

Received Date: 25 July 2024

Calibrated Date: 5 - 6 August 2024

Issued Date: 7 August 2024

Calibrated by: Ms. Juntaporn Kunhakom

Approved by:

(Mr. Sittichai Swaksuriyawong)
Group Manager

This report was prepared electronically using applicable electronic signature. Printing or copy of file are considered as a copy of the document.

The reported uncertainty of measurement was based on standard uncertainty multiplied by a coverage factor (k) providing a level of confidence of approximately 95%. This certificate may not be reproduced other than in full except with the prior written approval of the Electrical and Electronics Institute, Foundation for Industrial Development.

Page 1 of 6

เอกสารไม่ควบคุม

F-CAL-004 Ed.1



ELECTRICAL AND ELECTRONICS INSTITUTE
FOUNDATION FOR INDUSTRIAL DEVELOPMENT

Certificate No.: CP20240290EA

Calibration Report

Equipment: Sound Level Meter

Manufacturer: Larson Davis (Meter), PCB (Microphone), PCB (Preamplifier)

Model/Type: LxT1 (Meter), 377B02 (Microphone), PRMLxT1 (Preamplifier)

Serial No.: 0007306 (Meter), 345235 (Microphone), 077641 (Preamplifier)

ID No.: UAE.EFM.039/2566

Ambient Temperature: (23 ± 2) °C

Relative Humidity: (50 ± 15) %

Pressure: (101.3 ± 1.5) kPa

Method of Calibration :-
IEC 61672-3:2013.

Condition of this result of calibration

1. Reference standards instrument :-

Instrument	Model	Serial No.	Cert. No.	Due Date
1) Standard microphone	4180	2787490	AA-1012-23	12 November 2024
2) Arbitrary Function Generator	AFG2021	C010063	CK20240048EA	23 June 2025
3) Programmable Attenuator	PA5	2755	EF-0040-23	1 October 2024
4) 6.5 Digit precision multimeter	8846A	9610014	CB20230200EA	15 November 2024
5) Pressure humidity and Temperature Transmitter	PTU301	L3950483	CL1-P240023 CD20240142EA	24 March 2025 12 June 2025
6) Pressure humidity and Temperature Transmitter	PTU301	L3950484	CL1-P240030 CD20240143EA	11 April 2025 12 June 2025
7) Performance Audio Analyzer	U8903B	MY56510003	CB20240035EB CK20230072EA	13 February 2025 13 September 2024

2. This result of calibration was found accurate as shown on date and place of calibration only.

3. This certification is traceable to the international system of unit maintained at :-

Reference standards instrument for Acoustic function

- National Institute of Metrology (Thailand)

Reference standards instrument for Electrical function

- National Institute of Metrology (Thailand)

- Electrical and Electronics Institute; NSC Accredited Calibration No.0119

Result of Calibration:-

Function : 1. Indication at the calibration check frequency

Reference Acoustic Signal (dB)	Measured value (dB)	Deviation (dB)	Acceptance limits (dB)
-	-	-	-

Page 2 of 6

F-CAL-005 Ed.1

เอกสารไม่ควบคุม



ELECTRICAL AND ELECTRONICS INSTITUTE
FOUNDATION FOR INDUSTRIAL DEVELOPMENT

Certificate No.: CP20240290EA

Calibration Report

Function : 2. Self-generated Noise

2.1 Microphone Installed

Measured value (dB)
28.8

2.2 Microphone replaced by the electrical input signal device

Frequency Weighting	Measured value (dB)
A-weighting	28.7
C-weighting	28.4
Z-weighting	34.5

Function : 3. Acoustical signal tests of frequency weightings (Without Windscreen)

Meter free-field acoustic response at a level of 84 dB.

Frequency (Hz)	Deviation from various Frequency Weighting Response Curve			
	C-Weighting (dB)	A-Weighting (dB)	Z-Weighting (dB)	Acceptance limits (dB)
125	0.1	0.0	0.0	±1.0
1000	-0.1	-0.1	-0.1	±0.7
8000	-0.4	-0.5	-0.4	+1.5; -2.5

Function : 4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various Frequency Weighting Response Curve			
	C-Weighting (dB)	A-Weighting (dB)	Z-Weighting (dB)	Acceptance limits (dB)
63	0.0	0.0	0.0	±1.0
125	0.0	0.0	0.0	±1.0
250	0.0	0.0	0.0	±1.0
500	0.0	0.0	0.0	±1.0
1000	0.0	0.0	0.0	±0.7
2000	0.0	0.0	0.0	±1.0
4000	0.0	0.0	0.0	±1.0
8000	-0.1	-0.1	0.0	+1.5; -2.5
16000	0.0	0.0	0.0	+2.5; -16.0

เอกสารไม่ควบคุม

Page 3 of 6

F-CAL-005 Ed.1



ELECTRICAL AND ELECTRONICS INSTITUTE
FOUNDATION FOR INDUSTRIAL DEVELOPMENT

Certificate No.: CP20240290EA

Calibration Report

Function : 5. Frequency and time weighting at 1 kHz

5.1 Frequency weighting at 1 kHz

Frequency Weighting	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
C-weighting	94.0	0.0	±0.2
A-weighting	94.0	0.0	±0.2
Z-weighting	94.0	0.0	±0.2

5.2 Time weighting at 1 kHz

Time Weighting	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
Fast	94.0	0.0	±0.1
Slow	94.0	0.0	±0.1
LAeq	94.0	0.0	±0.1

Function : 6. Long-Term Stability

Long-term stability over 30 minutes, with steady 1 kHz signal at reference level.

Time Period to Apply Signal (min)	Reference SPL (dB)	Record SPL at Conclusion of Time Period (dB)	Deviated value (dB)	Acceptance limits (dB)
30	94.0	94.0	0.0	±0.1

Function : 7. Level Linearity on the reference level range

7.1 Level Linearity on the reference level range, Upper

Anticipated Value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
94.0	94.0	0.0	±0.8
99.0	99.0	0.0	±0.8
104.0	104.0	0.0	±0.8
109.0	109.0	0.0	±0.8
114.0	114.0	0.0	±0.8
119.0	119.0	0.0	±0.8
124.0	124.0	0.0	±0.8
129.0	129.0	0.0	±0.8
134.0	134.0	0.0	±0.8
139.0	139.0	0.0	±0.8
140.0	140.0	0.0	±0.8

เอกสารไม่ควบคุม

Page 4 of 6

F-CAL-005 Ed.1

Certificate No.: CP20240290EA

Calibration Report

7.2 Level Linearity on the reference level range, Lower

Anticipated Value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
94.0	94.0	0.0	±0.8
89.0	89.0	0.0	±0.8
84.0	84.0	0.0	±0.8
79.0	79.0	0.0	±0.8
74.0	74.0	0.0	±0.8
69.0	69.0	0.0	±0.8
64.0	64.0	0.0	±0.8
59.0	59.0	0.0	±0.8
54.0	54.0	0.0	±0.8
49.0	49.0	0.0	±0.8
44.0	44.1	0.1	±0.8
39.0	39.4	0.4	±0.8

Function : 8. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
Fast	200	136.0	0.0	±0.5
	2	118.8	-0.2	+1.0 ; -1.5
	0.25	109.7	-0.3	+1.0 ; -3.0
Slow	200	129.5	-0.1	±0.5
	2	109.8	-0.2	+1.0 ; -3.0
	200	130.0	0.0	±0.5
LAE	2	110.0	0.0	+1.0 ; -1.5
	0.25	100.9	-0.1	+1.0 ; -3.0

Function : 9. Peak C sound level

Number of cycles in test signal	Anticipated Value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
Complete cycle	135.4	134.8	-0.6	±2.0
Positive half cycle	134.4	134.0	-0.4	±1.0
Negative half cycle	134.4	134.0	-0.4	±1.0

Page 5 of 6

F-CAL-005 Ed.1

เอกสารไม่ควบคุม

Certificate No.: CP20240290EA

Calibration Report

Function : 10. Overload indication

Measured value (dB)		Deviated value (dB)	Acceptance limits (dB)
Positive one-half cycle	Negative one-half cycle		
142.6	142.6	0.0	±1.5

Function : 11. High-Level Stability

High-level stability over 5 minutes, with steady 1 kHz signal, 1 dB below upper boundary.

Time Period to Apply Signal (min)	Reference SPL (dB)	Record SPL at Conclusion of Time Period (dB)	Deviated value (dB)	Acceptance limits (dB)
5	139.0	139.0	0.0	±0.1

Uncertainty of measurement

Function	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1) Indication at the calibration check frequency	0.30	Not applicable
2) Self-generated Noise	0.10	Not applicable
3) Acoustical signal tests of frequency weightings - Free-field sound pressure response level	0.30	0.60 (10Hz to 4kHz) 0.70 (>4kHz to 10kHz)
4) Electrical signal tests of frequency weightings	0.20	0.20
5) Frequency and time weighting at 1 kHz	0.20	0.20
6) Long-Term Stability	0.10	0.10
7) Level Linearity on the reference level range	0.30	0.30
8) Tone burst response	0.20	0.30
9) Peak C sound level	0.20	0.35
10) Overload indication	0.20	0.25
11) High-Level Stability	0.10	0.10

Remarks:

1. Indication at the calibration check frequency can not measured because customer does not provide a sound calibrator.
2. The acceptance limit is for the deviated value.
3. Acceptance limits was IEC61672-3:2013 Class 1.
4. The coverage factor $k = 2.00$

- - End of Report - -

Page 6 of 6

F-CAL-005 Ed.1

เอกสารไม่ควบคุม

Certificate No.: CP20240322EA
Operation No.: CP2024080293

Certificate of Calibration

Equipment: Sound Level Meter

Manufacturer: Larson Davis (Meter), PCB (Microphone), PCB (Preamplifier)

Model/Type: LxT1 (Meter), 377B02 (Microphone), PRMLxT1 (Preamplifier)

Serial No.: 0007308 (Meter), 345238 (Microphone), 077643 (Preamplifier)

ID No.: UAE.EFM.040/2566

Customer: United Analyst and Engineering Consultant Co.,Ltd.


Address: 81 Soi Udomsuk 41, Sukhumvit Road, Bangchak Phrakhanong, Bangkok 10260

Received Date: 9 August 2024

Calibrated Date: 22 - 26 August 2024

Issued Date: 28 August 2024

Calibrated by: Ms. Juntaporn Kunhakom

Approved by: 
(Mr. Sittichai Swaksuriyawong)
Group Manager

This report was prepared electronically using applicable electronic signature. Printing or copy of file are considered as a copy of the document.

The reported uncertainty of measurement was based on standard uncertainty multiplied by a coverage factor (k) providing a level of confidence of approximately 95%. This certificate may not be reproduced other than in full except with the prior written approval of the Electrical and Electronics Institute, Foundation for Industrial Development.

Page 1 of 6

เอกสารไม่ควบคุม

F-CAL-004 Ed.1

Certificate No.: CP20240322EA

Calibration Report

Equipment: Sound Level Meter

Manufacturer: Larson Davis (Meter), PCB (Microphone), PCB (Preamplifier)

Model/Type: LxT1 (Meter), 377B02 (Microphone), PRMLxT1 (Preamplifier)

Serial No.: 0007308 (Meter), 345238 (Microphone), 077643 (Preamplifier)

ID No.: UAE.EFM.040/2566

Ambient Temperature: $(23 \pm 2) ^\circ\text{C}$

Relative Humidity: $(50 \pm 15) \%$

Pressure: $(101.3 \pm 1.5) \text{ kPa}$

Method of Calibration :- IEC 61672-3:2013.

Condition of this result of calibration

1. Reference standards instrument :-

Instrument	Model	Serial No.	Cert. No.	Due Date
1) Standard microphone	4180	2787490	AA-1012-23	12 November 2024
2) Arbitrary Function Generator	AFG2021	C010063	CK20240048EA	23 June 2025
3) Programmable Attenuator	PA5	2755	EF-0040-23	1 October 2024
4) 6.5 Digit precision multimeter	8846A	9610014	CB20230200EA	15 November 2024
5) Pressure humidity and Temperature Transmitter	PTU301	L3950483	CL1-P240023 CD20240142EA	24 March 2025 12 June 2025
6) Pressure humidity and Temperature Transmitter	PTU301	L3950484	CL1-P240030 CD20240143EA	11 April 2025 12 June 2025
7) Performance Audio Analyzer	U8903B	MY56510003	CB20240035EB CK20230072EA	13 February 2025 13 September 2024

2. This result of calibration was found accurate as shown on date and place of calibration only.

3. This certification is traceable to the international system of unit maintained at :-

Reference standards instrument for Acoustic function

- National Institute of Metrology (Thailand)

Reference standards instrument for Electrical function

- National Institute of Metrology (Thailand)
- Electrical and Electronics Institute; NSC Accredited Calibration No.0119

Result of Calibration:-

Function : 1. Indication at the calibration check frequency

Reference Acoustic Signal (dB)	Measured value (dB)	Deviation (dB)	Acceptance limits (dB)
-	-	-	-

Page 2 of 6

F-CAL-005 Ed.1

เอกสารไม่ควบคุม

Certificate No.: CP20240322EA

Calibration Report

Function : 2. Self-generated Noise

2.1 Microphone Installed

Measured value (dB)
29.4

2.2 Microphone replaced by the electrical input signal device

Frequency Weighting	Measured value (dB)
A-weighting	29.0
C-weighting	28.9
Z-weighting	35.5

Function : 3. Acoustical signal tests of frequency weightings (Without Windscreen)

Meter free-field acoustic response at a level of 84 dB.

Frequency (Hz)	Deviation from various Frequency Weighting Response Curve			
	C-Weighting (dB)	A-Weighting (dB)	Z-Weighting (dB)	Acceptance limits (dB)
125	0.2	0.1	0.2	±1.0
1000	0.3	0.3	0.3	±0.7
8000	-0.6	-0.5	-0.5	+1.5; -2.5

Function : 4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various Frequency Weighting Response Curve			
	C-Weighting (dB)	A-Weighting (dB)	Z-Weighting (dB)	Acceptance limits (dB)
63	-0.1	0.1	0.0	±1.0
125	0.0	0.0	-0.1	±1.0
250	-0.1	0.0	0.0	±1.0
500	0.0	0.0	-0.1	±1.0
1000	0.0	0.0	0.0	±0.7
2000	0.0	0.0	0.0	±1.0
4000	0.0	-0.1	0.0	±1.0
8000	-0.1	-0.1	0.0	+1.5; -2.5
16000	0.0	0.0	-0.1	+2.5; -16.0

เอกสารไม่ควบคุม

Page 3 of 6

F-CAL-005 Ed.1

Certificate No.: CP20240322EA

Calibration Report

Function : 5. Frequency and time weighting at 1 kHz

5.1 Frequency weighting at 1 kHz

Frequency Weighting	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
C-weighting	94.0	0.0	±0.2
A-weighting	94.0	0.0	±0.2
Z-weighting	94.0	0.0	±0.2

5.2 Time weighting at 1 kHz

Time Weighting	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
Fast	94.0	0.0	±0.1
Slow	94.0	0.0	±0.1
LAeq	94.0	0.0	±0.1

Function : 6. Long-Term Stability

Long-term stability over 30 minutes, with steady 1 kHz signal at reference level.

Time Period to Apply Signal (min)	Reference SPL (dB)	Record SPL at Conclusion of Time Period (dB)	Deviated value (dB)	Acceptance limits (dB)
30	94.0	94.0	0.0	±0.1

Function : 7. Level Linearity on the reference level range

7.1 Level Linearity on the reference level range, Upper

Anticipated Value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
94.0	94.0	0.0	±0.8
99.0	99.0	0.0	±0.8
104.0	104.0	0.0	±0.8
109.0	109.0	0.0	±0.8
114.0	114.0	0.0	±0.8
119.0	119.0	0.0	±0.8
124.0	124.0	0.0	±0.8
129.0	129.0	0.0	±0.8
134.0	134.0	0.0	±0.8
139.0	139.0	0.0	±0.8
140.0	140.0	0.0	±0.8

เอกสารไม่ควบคุม

Page 4 of 6

F-CAL-005 Ed.1

Certificate No.: CP20240322EA

Calibration Report

7.2 Level Linearity on the reference level range, Lower

Anticipated Value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
94.0	94.0	0.0	±0.8
89.0	89.0	0.0	±0.8
84.0	84.0	0.0	±0.8
79.0	79.0	0.0	±0.8
74.0	74.0	0.0	±0.8
69.0	69.0	0.0	±0.8
64.0	64.0	0.0	±0.8
59.0	59.0	0.0	±0.8
54.0	54.0	0.0	±0.8
49.0	49.0	0.0	±0.8
44.0	44.1	0.1	±0.8
39.0	39.4	0.4	±0.8

Function : 8. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
Fast	200	135.9	-0.1	±0.5
	2	118.8	-0.2	+1.0; -1.5
	0.25	109.6	-0.4	+1.0; -3.0
Slow	200	129.5	-0.1	±0.5
	2	109.8	-0.2	+1.0; -3.0
	200	130.0	0.0	±0.5
LAE	2	110.0	0.0	+1.0; -1.5
	0.25	100.8	-0.2	+1.0; -3.0

Function : 9. Peak C sound level

Number of cycles in test signal	Anticipated Value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
Complete cycle	135.4	134.8	-0.6	±2.0
Positive half cycle	134.4	134.0	-0.4	±1.0
Negative half cycle	134.4	134.1	-0.3	±1.0

เอกสารไม่ควบคุม

Page 5 of 6

F-CAL-005 Ed.1

Certificate No.: CP20240322EA

Calibration Report

Function : 10. Overload indication

Measured value (dB)		Deviated value (dB)	Acceptance limits (dB)
Positive one-half cycle	Negative one-half cycle		
143.0	142.8	-0.2	±1.5

Function : 11. High-Level Stability

High-level stability over 5 minutes, with steady 1 kHz signal, 1 dB below upper boundary.

Time Period to Apply Signal (min)	Reference SPL (dB)	Record SPL at Conclusion of Time Period (dB)	Deviated value (dB)	Acceptance limits (dB)
5	139.0	139.0	0.0	±0.1

Uncertainty of measurement

Function	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1) Indication at the calibration check frequency	0.30	Not applicable
2) Self-generated Noise	0.10	Not applicable
3) Acoustical signal tests of frequency weightings - Free-field sound pressure response level	0.30	0.60 (10Hz to 4kHz) 0.70 (>4kHz to 10kHz)
4) Electrical signal tests of frequency weightings	0.20	0.20
5) Frequency and time weighting at 1 kHz	0.20	0.20
6) Long-Term Stability	0.10	0.10
7) Level Linearity on the reference level range	0.30	0.30
8) Tone burst response	0.20	0.30
9) Peak C sound level	0.20	0.35
10) Overload indication	0.20	0.25
11) High-Level Stability	0.10	0.10

Remarks:

1. Indication at the calibration check frequency can not measured because customer does not provide a sound calibrator.
2. The acceptance limit is for the deviated value.
3. Acceptance limits was IEC61672-3:2013 Class 1.
4. The coverage factor $k = 2.00$

- - End of Report - -

เอกสารไม่ควบคุม

Page 6 of 6

F-CAL-005 Ed.1



Certificate of Calibration

Cert.No.: 24CH1422
Page.: 1 of 3

Equipment : pH Meter
Manufacturer : EcoSense
Model : pH100A
Serial No. : 24H005160JEN
ID No. : UAE.EFM.042/2567 (EFM,pH.05/67)
Condition As-Received: Used Item
Received Date : 13 November 2024
Calibration Date : 14-15 November 2024
Reference : 2411-0421WSC-5
Submitted by : United Analyst and Engineering Consultant Co.,Ltd.
3 Soi Udomsuk 41, Sukhumvit Road,
Bangchak, Phrakhanong, Bangkok 10260

Ambient Temperature : (25 ± 2.5) °C
Relative Humidity : (50 ± 15) %
Calibration Procedure : In - house method :
- CP-CH5 by direct measurement with DC voltage
standard and direct measurement with
certified reference material (CRM)
- CP-CH8 by comparison with temperature standard
11/14/2025 12:00:00 AM

Calibrated by : Warakorn Lernagatrakul

Approved by :
Approved Signatory

() Unnopphol Harachai
() Ponpan Paipim
(✓) Saitip Meangmai

Issue Date : 20 November 2024

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

เอกสารไม่ควบคุม



Cert.No.: 24CH1422
Page.: 2 of 3

Condition of this calibration result

Instrument	Serial No.	ID No.	Cert. No.	Due Date
1) Document Process Calibrator	54030049	130RC116	24E2759	25 Aug 2025
2) Ref. Standard Thermometer	4982054	110RC044	24I757	14 Jul 2025

- This Certification is traceable to SI Through Technology Promotion Association (Thailand - Japan)

2. Certified Reference Materials : The measurement results are traceable to SI through Hach Lenge GmbH Ltd.,
Deutsche Akkreditierungsstelle, Accredited No.D-RM-15184-01-00
: The measurement results are traceable to SI through CPA chem Ltd.,
ANSI-ASQ National Accreditation Board, Accredited No. AR-1835

Buffer Solution	Manufacturer	Lot No.	Exp. date
pH 4.008	CPA chem	1034203	27 Sep 2026
pH 6.999	Hach Lenge GmbH	C03145	28 Feb 2026
pH 10.010	CPA chem	1034205	27 Sep 2025

3. This certificate is valid only to the item calibrated on date and place of calibration.

Calibration Results

Function : mV Measurement

Performing standard curve by Document Process Calibrator at pH (4,7)(7,10)

Unit Under Calibration	Nominal Value	Standard Voltage Input	Actual Reading		Uncertainty of Measurement (± mV)	Coverage factor k
	pH	mV	mV	pH		
pH Meter S/N.: 24H005160JEN	4.00	177.48	177	4.01	0.58	2.00
	7.00	0.00	0	7.00	0.58	2.00
	7.00	0.00	0	7.00	0.58	2.00
	10.00	-177.48	-177	10.01	0.58	2.00

เอกสารไม่ควบคุม



Cert.No.: 24CH1422
Page.: 3 of 3

Calibration Results

Function : pH Measurement

Performing three buffers standard curve by using buffer nominal pH (4,7)(7,10)

Unit Under Calibration	Standard pH Buffer Solution	Actual pH Reading	Actual mV Reading (mV)	Uncertainty of pH Measurement (±)	Coverage factor k
pH Electrode S/N.: 240904SIA605377	4.008	4.01	173	0.0071	2.00
	6.999	7.00	0	0.0092	2.00
	6.999	7.00	0	0.0085	2.00
	10.010	10.01	-173	0.0085	2.00

Function : Temperature Measurement

(*) Without adjustment

This equipment was connected with Temperature Probe;

- Model : -

- Serial No. : 240904SIA605377

Dimension of probe

- Length : 110 mm.

- Diameter : 12 mm.

- Immersion Depth : 100 mm.

Calibration Point (°C)	Standard Temperature (°C)	UUC* Reading (°C)	Error (°C)	Uncertainty of measurement (± °C)	Coverage factor k
15.0	15.002	15.1	0.098	0.13	2.00
30.0	30.002	30.0	-0.002	0.13	2.00
45.0	45.003	44.8	-0.203	0.13	2.00

Remark : - UUC* = Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k, providing a level of confidence of approximately 95 %.

-00-

เอกสารไม่ควบคุม



Certificate of Testing

Cert.No.: 24TW241
Page.: 1 of 2

Equipment : DO Meter
Manufacturer : Horiba
Model : LAQUA-DO210
Serial No. : HEOL0004
ID No. : UAE.EFM.087/2564 (EFM.DO.06/64)
Received Date : 05 November 2024
Test Date : 06 November 2024
Reference : 2411-0123WSC-3
Submitted by : United Analyst and Engineering Consultant Co.,Ltd.
3 Soi Udomsuk 41, Sukhumvit Road, Bangchak,
Phrakhanong, Bangkok 10260

Laboratory Condition : Temperature (25 ± 5) °C
Humidity (50 ± 20) %
Test Procedure : In - house method : CP-CH9
by Comparison Technique with Azide Modification Method

Tested by : Walalak Sirithean

Approved by :
Approved Signatory

() Unnopphol Harachai
() Ponpan Paipim
(✓) Saitip Meangmai

Issue Date : 9 November 2024

เอกสารไม่ควบคุม



Cert.No.: 24TW241
Page.: 2 of 2

Condition of this result of calibration

1. Reference Standard Instruments :
This certification is traceable to the International System of Unit through the reference standards laboratory of Industrial Calibration Center, Technology Promotion Association (Thailand-Japan).

Instruments	Serial No.	ID No.	Certificate No.	Due Date
1. Burette	-	130BU10	23CG1172	22 Mar 2025
2. Balance	14233821	110RC001	24MM131	04 July 2025

2. Standard Material :-

Material	Manufacturer	Lot.No.	Assay
Sodium Thiosulfate 5-Hydrate AR	KEMAUS	2203162447	99.6%

Result : Dissolved Oxygen Meter Adjustment With Air 100 %
Dissolved Oxygen Probe No.: 9K0E0257

Titration Method (Azide Modification Method)	DO Meter Reading	Standard Deviation
(mg/L)	(mg/L)	(mg/L)
8.20	8.19	0.0084

This report was certified only for the instrument we tested. It is allowable to use for study
Intend to use for advertising and referral purpose is prohibited. This report may not be reproduced
other in full, without written approval of the laboratory

-o0o-

เอกสารไม่ควบคุม



Equipment : DO Meter with Sensor
Condition As-Received : Used Item
Reference : 2411-0123WSC-4
Procedure Used :-

Cert. No.: 24LM173
Page.: 2 of 2

Calibration were conducted using in-house calibration procedure CP-OT01 according to comparison with Industrial Platinum Resistance Thermometer (IPRT) into Temperature Bath.
The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

Instrument	Serial No.	Cert. No.	Traceable	Due Date
1) Digital Thermometer	3240076	241317	TPA	21 Mar 2025

2. This certificate is valid only to the item calibrated on date and place of calibration.
3. This certification is traceable to the International System of Unit.

Remark : TPA : Technology Promotion Association (Thailand - Japan)

Result of Calibration :- (*) Without Adjustment

Function : Temperature measurement.

This instrument was connected with temperature sensor, S/N.: 9K0E0257

Calibration Point (°C)	Immersion Depth (mm)	Standard Temperature (°C)	UUC* Reading (°C)	Error (°C)	Uncertainty (± °C)	Coverage Factor k
15.0	100	15.002	15.0	-0.002	0.16	2.00
30.0	100	30.003	30.0	-0.003	0.16	2.00
45.0	100	45.003	45.0	-0.003	0.16	2.00

UUC* : Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

เอกสารไม่ควบคุม



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL.0-2717-3000-29 FAX.0-2719-9484



Certificate of Calibration

Cert. No.: 24LM173
Page.: 1 of 2

Equipment : DO Meter with Sensor
Manufacturer : Horiba
Model : LAQUA-DO210
Serial No. : HEOL0004
ID No. : UAE.EFM.087/2564(EFM.DO.06/64)
Submitted by : United Analyst and Engineering Consultant Co.,Ltd.
3 Soi Udomsuk 41, Sukhumvit Road,
Bangchak, Phrakhanong, Bangkok 10260
Location : TPA On Site Calibration Laboratory
Received Order : 05 November 2024
Calibrated Date : 06 November 2024
Ambient Temperature : (26 ± 10) °C
Relative Humidity : (50 ± 30) %
AC Line Voltage : (220 ± 22) V

Calibrated by : Warakorn Lerngagtrakul

Approved by :

- () Ponpan Paipim
() Suwit Imjai
(✓) Kunchit Promprat

Issue Date : 07 November 2024

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

เอกสารไม่ควบคุม



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL.0-2717-3000-29 FAX.0-2719-9484



Certificate of Calibration

Cert.No.: 24CH1524
Page.: 1 of 3

Equipment : Conductivity Meter
Manufacturer : YSI Environmental
Model : Pro 30
Serial No. : 24J101890
ID No. : UAE.EFM.045/2567(EFM.SCT.01/67)
Condition As-Received : Used Item
Received Date : 04 December 2024
Calibration Date : 06 December 2024
Reference : 2412-0103WSC-3
Submitted by : United Analyst and Engineering Consultant Co.,Ltd.
3 Soi Udomsuk 41, Sukhumvit Road,
Bangchak, Phrakhanong, Bangkok 10260
Ambient Temperature : (25 ± 2.5) °C
Relative Humidity : (50 ± 15) %
Calibration Procedure : In -house method :
- CP-CH6 by direct measurement
with certified reference material (CRM)
- CP-CH8 by comparison with temperature standard

Calibrated by : Warakorn Lerngagtrakul

Approved by :

- () Unnopphol Harachai
() Ponpan Paipim
(✓) Saithip Meangmai

Issue Date : 06 December 2024

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

เอกสารไม่ควบคุม



Cert.No.: 24CH1524

Page.: 2 of 3

Condition of this result of calibration

1. Reference Standard Instrument :-

Instrument	Serial No.	ID No.	Certificate No.	Due date
1) Thermometer	1963878	130RC095	24I995	09 Sep 2025
2) Ref. Std. Thermometer	4982054	110RC044	24I757	14 July 2025

- This Certification is traceable to SI Throught Technology Promotion Association (Thailand - Japan)

2. Certified Reference Materials :-

- Conductivity calibration solution, CPA chem Ltd., The measurement results are traceable to SI through CPA chem Ltd., ANSI-ASQ National Accreditation Board, Accredited No. AR-1835

Conductivity Solution	Manufacturer	Lot No.	Exp. date
1412.9 μ S/cm	CPA Chem	1005307	15 June 2025
12.881 mS/cm	CPA Chem	1005308	15 June 2025

- Control Conductivity calibration solution temperature by Water bath (25 ± 0.1 °C)

3. This certificate is valid only to the item calibrated on date and place of calibration.

Calibration results

Function : Conductivity Measurement

(*) After Adjustment at 1412.9 μ S/cm

Conductivity Electrode Serial No.: 24B100382

Standard Conductivity Solution	Before Adjustment UUC* Reading	After Adjustment UUC* Reading	Uncertainty of Measurement (\pm)	Coverage factor k
1412.9 μ S/cm	1176 μ S/cm	1412 μ S/cm	9.2 μ S/cm	2.00
12.881 mS/cm	10.49 mS/cm	12.90 mS/cm	0.086 mS/cm	2.00

Remark : - UUC* = Unit Under Calibration



Cert.No.: 24CH1524

Page.: 3 of 3

Calibration Results

Function : Temperature Measurement

This equipment was connected with Temperature Probe;

- Model :	9383
- Serial No. :	24B100382

Dimension of probe;

- Length :	90 mm
- Diameter :	2.5 mm
- Immersion Depth :	80 mm

Calibration Result : Without adjustment

Calibration Point (°C)	Standard Temperature (°C)	UUC* Reading (°C)	Error (°C)	Uncertainty of Measurement (\pm °C)	Coverage factor k
15.0	15.003	14.9	-0.104	0.13	2.00
30.0	30.001	29.9	-0.101	0.13	2.00
45.0	45.006	44.9	-0.106	0.13	2.00

Remark : - UUC* = Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k, providing a level of confidence of approximately 95 %.

-000-

เอกสารไม่ควบคุม

เอกสารไม่ควบคุม

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7139 MOO 13, SOI SUTINAKORN 11 TAMBON BANG KAE, B.
AMPHOE BANG PHU SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL: 0600-2116-7800-1 FAX: 0600-2116-7140



Page 1 of 2

Certificate of Calibration

Customer

Name : UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.
Address : 81 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Prakanong, Bangkok 10260

Certificate No : 25-ACT-073
Request No : Req-2025-1017

Unit Under Calibration Details

Measurement item : Acoustic Calibrator Class : 2
Manufacturer : LARSON DAVIS Range : 94 , 114 dB / 1000 Hz
Model : CAL150 Instrument Status : Used
Serial Number : 6458
ID : UAE.EFM.056.2564

Calibration Environment and Details

Temperature : (23 ± 2 °C)
Humidity : (50 ± 20 %RH)
Barometric Pressure : (1013 ± 10.0 hPa)
Received Date : 9 May 2025
Calibration Date : 20 May 2025
Location of Calibration : LAB 1 Acoustic
Calibration Procedure : In-house method CP-ACT-02 based on IEC 60942:2017 Electroacoustics - Sound calibrators

Reference Standard	Model	Serial Number	Traceable	Due Calibration
Sound Calibrator	SV 35A	58079	EEL	12 June 2025
THD Multimeter	2015	1047763	NIMT	4 February 2026

Traceability : This certificate provides traceability of measurement to recognized national standard, and to the realization of the international System of Units (SI).

Note

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor $k=2$, providing a level of confidence approximately 95 %.

Calibrated By : Mr. Noppadon Luangart
Approved By : Mr. Pacit Mathavorn
Service Calibration Engineer
Calibration Engineer Supervisor
Issue Date : 20 May 2025

เอกสารไม่ควบคุม

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7139 MOO 13, SOI SUTINAKORN 11 TAMBON BANG KAE, B.
AMPHOE BANG PHU SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL: 0600-2116-7800-1 FAX: 0600-2116-7140



Page 2 of 2

Certificate No : 25-ACT-073

Request No : Req-2025-1017

Sound pressure level

Calibration Results : Without Adjustment

Calibration Range (dB)	Without Adjustment (dB)		Adjustment (dB)		Uncertainty (\pm dB)
	Measured	Deviated value	Measured	Deviated value	
94 dB / 1000 Hz	93.88	-0.12	-	-	0.12
114 dB / 1000 Hz	113.91	-0.09	-	-	0.11

Frequency of Sound pressure level

Calibration Range (Hz)	Without Adjustment		Adjustment		Uncertainty (\pm %)
	Measured (Hz)	Deviated value	Measured (Hz)	Deviated value	
94 dB / 1000 Hz	1000.0	0.00	-	-	0.01
114 dB / 1000 Hz	1000.0	0.00	-	-	0.010

Total Harmonic Distortion plus Noise of Sound pressure level (THD+N %)

Calibration Range (Hz)	Without Adjustment		Adjustment		Uncertainty (\pm %)
	Measured (%)		Measured (%)		
94 dB / 1000 Hz	1.30		-		0.17
114 dB / 1000 Hz	0.64		-		0.17

Note :

- The calibration results exclude the calibration pressure correction
- The calibration results exclude the microphone volume correction

End of Calibration

เอกสารไม่ควบคุม

Cert. No. : ACL25022
Pages : 1 of 8

Calibration Certificate

Equipment : SOUND LEVEL METER
Manufacturer : RION
Model : NL-42 / Microphone UC-52 / Preamplifier NH-24
Serial No.: 00408982 / 186172 / 00727
ID No.: UAE.EFM.009/2564

Condition As Found : GOOD

Customer : UNITED ANALYST AND ENGINEERING CONSULTANT (UAE)
81 SOL UDOMSUK 41, SUKHUMVIT ROAD,
BANGCHAK SUB-DISTRICT,
PHRAKHANONG DISTRICT, BANGKOK 10260
THAILAND.

Location : -
Ambient Temperature : (23.0 ± 3) °C
Pressure : (101.3 ± 3) kPa
Relative Humidity : (50.0 ± 20) %

Received Date : 03 JANUARY 2025
Calibration Date : 13 - 14 JANUARY 2025
Date of Issue : 15 JANUARY 2025

Calibrated by : Nathakorn Pisutpaisan

Approved by : 
(Thanakul Petchurai)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced
other than in full, except with the prior written approval of the head of Calibration Laboratory.

เอกสารไม่ควบคุม

Cert. No. : ACL25022
Job No. : VC68AC0056
Pages : 2 of 8

Calibration Procedure : CP-AC-01

Calibration Method :

This equipment was calibrated by follow on IEC-61672-3 (2013) Standard for sound level meter (SLM).
The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference
Standard Instruments.
For tests results of each items were made by observation of each Instruments display and also with SLM's display.

Condition of this result of calibration :

1. Reference Standard Instruments :

Instrument	Model	Serial No.	Cert. No.	Due Date
Waveform Generator	33210A	MY48017076	EF-0009-24	05-FEB-25
Waveform Generator	33511B	MY52302742	EF-0007-24	05-FEB-25
Digital Multimeter	33461A	MY53220104	EEL-BP 21/0267	13-FEB-25
Digital Multimeter	33461A	MY53220076	EEL-BP 20/0267	15-FEB-25
Digital Multimeter	34461A	MY60024273	EEL-BP 22/0267	15-FEB-25
Programmable Attenuator	MAT-1070	62100114	EF-0008-24	05-FEB-25
Condenser Microphone	4180	2977900	AA-1001-24	12-FEB-25
Measuring Amplifier	NA-42KAJ	34560495	AA-3001-24	05-FEB-25

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is traceable to the international system of unit maintained at :

- 3.1 National Institute of Metrology (Thailand),
- 3.2 Thailand Institute of Scientific and Technological Research (TISTR).

เอกสารไม่ควบคุม

Cert. No. : ACL25022
Job No. : VC68AC0056
Pages : 3 of 8

Summary of Measurement Result :

Parameter	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	0.2	N/A
2. Self-generated noise	0.2	N/A
3. Acoustical signal tests of frequency weightings		
125 Hz	0.3	0.6
1000 Hz	0.3	0.6
8000 Hz	0.3	0.7
4. Electrical signal tests of frequency weightings		
For 10 Hz to 4 kHz	0.3	0.6
For > 4 kHz to 10 kHz	0.3	0.7
For > 10 kHz to 20 kHz	0.3	1.0
5. Frequency and time weightings at 1 kHz	0.2	0.2
6. Long - term stability	0.1	0.1
7. Level linearity on the reference level range	0.2	0.3
8. Level linearity including the level range control	0.2	0.3
9. Tone burst response	0.2	0.3
10. Peak C sound level	0.2	0.35
11. Overload indication	0.2	0.25
12. High level stability	0.1	0.1

เอกสารไม่ควบคุม

Cert. No. : ACL25022
Job No. : VC68AC0056
Page : 4 of 8

Result of calibration :

1. Absolute sensitivity

Reference Acoustic Signal (dB)	Measured Value (dB)	Deviation (dB)	Acceptance Limit (dB)
93.9 (93.94)	93.9	0.0	±0.3

2. Self-generated noise

2.1 Normal test

Measured Value (dB)
14.6

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting (dB)	Weighting (dB)
A - weight	11.2
C - weight	17.1
Flat	22.9

3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
125	0.3	0.4	0.4	± 1.5
1000	0.2	0.2	0.2	± 1.0
8000	2.1	2.1	2.2	±5.0

เอกสารไม่ควบคุม

Cert. No. : ACL25022
Job No. : VC68AC0056
Pages : 5 of 8

4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	0.0	0.0	0.0	±2.0
125	0.1	0.1	0.0	±1.5
250	0.0	0.0	0.0	±1.5
500	0.0	0.1	0.0	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.1	0.0	±2.0
4000	0.0	0.0	0.0	±3.0
8000	0.0	0.1	0.1	±5.0

5. Frequency and time weightings at 1 kHz

5.1 Frequency weightings at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.2
C - weight	94.0	94.0	0.0	± 0.2
Flat	94.0	94.0	0.0	± 0.2

5.2 Time weighting at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	94.0	94.0	0.0	± 0.1
Slow	94.0	94.0	0.0	± 0.1
Leq	94.0	94.0	0.0	± 0.1

6. Long - term stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.1	0.1	± 0.2

เอกสารไม่ควบคุม

Cert. No. : ACL25022
Job No. : VC68AC0056
Pages : 6 of 8

7. Level linearity on the reference level range

Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
137.0	137.0	0.0	± 1.1
136.0	136.0	0.0	± 1.1
135.0	135.0	0.0	± 1.1
134.0	134.0	0.0	± 1.1
133.0	133.0	0.0	± 1.1
132.0	132.0	0.0	± 1.1
131.0	131.0	0.0	± 1.1
129.0	129.0	0.0	± 1.1
124.0	124.0	0.0	± 1.1
119.0	119.0	0.0	± 1.1
114.0	114.0	0.0	± 1.1
109.0	109.0	0.0	± 1.1
104.0	104.0	0.0	± 1.1
99.0	99.0	0.0	± 1.1
94.0	94.0	0.0	± 1.1
89.0	89.0	0.0	± 1.1
84.0	84.0	0.0	± 1.1
79.0	79.0	0.0	± 1.1
74.0	74.0	0.0	± 1.1
69.0	69.0	0.0	± 1.1
64.0	64.0	0.0	± 1.1
59.0	59.0	0.0	± 1.1
54.0	54.0	0.0	± 1.1
49.0	49.0	0.0	± 1.1
44.0	44.0	0.0	± 1.1
39.0	39.0	0.0	± 1.1
34.0	34.0	0.0	± 1.1
30.0	30.0	0.0	± 1.1
29.0	29.0	0.0	± 1.1
28.0	28.0	0.0	± 1.1
27.0	27.1	0.1	± 1.1
26.0	26.0	0.0	± 1.1
25.0	25.1	0.1	± 1.1

เอกสารไม่ควบคุม

Cert. No. : ACL25022
Job No. : VC68AC0056
Pages : 7 of 8

8. Level linearity including the level range control

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
130	94.0	94.0	0.0	±1.1

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
130	29.0	28.9	-0.1	±1.1

9. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Cycle	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.1	0.1	±1.0
Slow	2	8	108.0	108.0	0.0	1.5 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
SEL	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
	2	8	108.0	108.1	0.1	1.0 ; -2.5
	200	800	128.0	128.1	0.1	±1.0

เอกสารไม่ควบคุม

Cert. No. : ACL25022
Job No. : VC68AC0056
Pages : 8 of 8

10. Peak C sound level

Number of cycle in test signal	Anticipated Value (dB)	Measured Value, L _{peak} (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	130.0	130.0	0.0	±3.0
One	133.4	133.4	0.0	±3.0

Number of cycle in test signal	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	±2.0
Positive half cycle	135.4	135.1	-0.3	±2.0
Negative half cycle	135.4	135.1	-0.3	±2.0

11. Overload indication

Measured value (dB)		Deviated Value (dB)	Acceptance Limits (dB)
Positive one-half cycle	Negative one-half cycle		
89.5	89.5	0.0	±1.5

12. High level stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor $k = 2$
or any value following calculation, providing a level of confidence of approximately 95 %

End of Calibration Certificate

เอกสารไม่ควบคุม

Certificate of Calibration

Customer

Name : UNITED ANALYST AND ENGINEERING CONSULTANT CO., LTD.
Address : 81 Soi Udomsak 41, Sukhumvit Road, Bangchak, Prakanong, Bangkok 10260

Certificate No : 25-SLM-108
Request No : Req-2025-0595

Unit Under Calibration Details

Measurement Item : Sound Level Meter
Manufacturer : RION
Model : NL-42
Serial Number : 00405983
ID : UAE EFM 010/2568
Resolution : 0.1 dB

Microphone Class : 2
Microphone Model : UC-52
Microphone S/N : 186173
Preamplifier Model : NH-24
Preamplifier S/N : 90428
Instrument Status : Used

Calibration Environment and Details

Temperature : 23 °C ± 2 °C
Humidity : 50 %RH ± 20 %RH
Barometric Pressure : 1013 hPa ± 10 hPa
Received Date : 5 March 2025
Calibrated Date : 18 March 2025
Calibration Procedure : In-house method CP-SLM-01 based on IEC 61672-3 : 2013 Electroacoustics - Sound level meters - Part 3: Periodic tests
Location of Calibration : Lab Acoustic

Instrument	Brand	Model	S/N	Due calibration	Traceability
Standard Microphone	Briel & Kjaer	4192	2294985	25 June 2025	SIMT
Audio Generator	SvanteK	Svan401	131	15 October 2025	WK Electric

Note :
The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor $k = 2$, providing a level of confidence approximately 95 %.

Calibrated By : 
Mr. Neppadon Luangrat
Service Calibration Engineer

Approved By : 
Mr. Pait Mahavorn
Calibration Engineer Supervisor

Issue Date : 18 March 2025

Certificate No : 25-SLM-108
Request No : Req-2025-0595

1. Indication at the calibration check frequency

UUC Setting	Nominal	Before Adjust		After Adjust		UNCERTAINTY (± dB)	Acceptance Limit (± dB)	Result
		UUC	ERR	UUC	ERR			
FAST / A / 30-130	Level	(dB)	(dB)	(dB)	(dB)			
Calibrator Setting	(dB)	(dB)	(dB)	(dB)	(dB)			
1000 Hz 114 dB	114.03	114.0	-0.03	114.0	-0.03	0.20	0.30	Pass

Note : Absolute sensitivity was established by the use of Sound Calibrator Brand SVANTER, Model SV 35, SN.44792

2. Self-generated noise, Microphone installed

UUC Setting	Measured	UNCERTAINTY
FAST / 30-130		
UUC Weighting	(dB)	(± dB)
A	16.3	0.10

3. Self-generated noise, Microphone replaced by the electrical input signal device

UUC Setting	Measured	UNCERTAINTY
FAST / 30-130		
UUC Weighting	(dB)	(± dB)
A	12.6	0.10
C	17.0	0.10
Z	20.1	0.10

4. Acoustic signal test of frequency weightings (Without Windscreen)

UUC Setting	Deviation from various Frequency Weighting Response curve			UNCERTAINTY (± dB)	Acceptance Limit (± dB)	Result
	A	C	Z			
FAST / 30-130	(dB)	(dB)	(dB)			
STD Setting	(dB)	(dB)	(dB)			
125 Hz	0.2	0.4	0.4	0.60	1.5	Pass
1000 Hz	0.0	0.0	0.0	0.60	1.0	Pass
4000 Hz	1.1	1.1	1.1	0.60	3.0	Pass
8000 Hz	0.4	0.4	0.3	0.70	5.0	Pass

Certificate No : 25-SLM-108
Request No : Req-2025-0595

5. Electrical signal test of frequency weightings, Weighting network response with relative to 1 kHz

UUC Setting	Deviation from various Frequency Weighting Response curve			UNCERTAINTY (± dB)	Acceptance Limit (± dB)	Result
	A (dB)	C (dB)	Z (dB)			
FAST / 30-130						
STD Setting	(dB)	(dB)	(dB)			
63 Hz	-0.2	0.0	-0.1	0.20	2.0	Pass
125 Hz	-0.1	0.0	0.0	0.20	1.5	Pass
250 Hz	-0.1	0.0	0.0	0.20	1.5	Pass
500 Hz	0.0	0.0	0.0	0.20	1.5	Pass
1000 Hz	0.0	0.0	0.0	0.20	1.0	Pass
2000 Hz	0.0	0.1	0.0	0.20	2.0	Pass
4000 Hz	0.0	0.0	0.0	0.20	3.0	Pass
8000 Hz	0.1	0.1	0.0	0.20	5.0	Pass
16000 Hz	-1.3	-1.4	0.0	0.20	>5, <INF	Pass

6. Frequency and time weightings at 1kHz

UUC Setting	STD	Measured		UNCERTAINTY (± dB)	Acceptance Limit (± dB)	Result
		REF	ERR			
FAST / 30-130						
UUC Weighting	(dB)	(dB)	(dB)			
A	114.00	114.0	0.0	0.20	0.20	Pass
C	114.00	114.0	0.0	0.20	0.20	Pass
Z	114.00	114.0	0.0	0.20	0.20	Pass

UUC Setting	STD	Measured		UNCERTAINTY (± dB)	Acceptance Limit (± dB)	Result
		REF	ERR			
30-130 / A						
UUC Time Response	(dB)	(dB)	(dB)			
Fast	114.00	114.0	0.0	0.20	0.10	Pass
Slow	114.00	114.0	0.0	0.20	0.10	Pass
Log	114.00	114.0	0.0	0.20	0.10	Pass

Certificate No : 25-SLM-108
Request No : Req-2025-0595

7. Long Term Stability

UUC Setting	Measured	UNCERTAINTY (± dB)	Acceptance Limit (± dB)	Result
FAST / A / 30-130	UUC			
STD Setting	(dB)			
Initial	114.0			
Final	114.0			
Deviated	0.0	0.10	0.30	Pass

8. Level linearity on the reference level range

UUC Setting	Anticipated	Deviation		UNCERTAINTY (± dB)	Acceptance Limit (± dB)	Result
FAST / A / 30-130	REF	UUC	ERR			
STD dB	(dB)	(dB)	(dB)			
130.00	130	137.9	-0.1	0.30	1.1	Pass
134.00	134	134.0	0.0	0.30	1.1	Pass
129.00	129	129.9	-0.1	0.30	1.1	Pass
124.00	124	123.9	-0.1	0.30	1.1	Pass
119.00	119	119.0	0.0	0.30	1.1	Pass
114.00	114	114.0	0.0	0.30	1.1	Pass
109.00	109	109.0	0.0	0.30	1.1	Pass
104.00	104	104.0	0.0	0.30	1.1	Pass
99.00	99	99.0	0.0	0.30	1.1	Pass
94.00	94	94.0	0.0	0.30	1.1	Pass
89.00	89	89.0	0.0	0.30	1.1	Pass
84.00	84	84.0	0.0	0.30	1.1	Pass
79.00	79	79.0	0.0	0.30	1.1	Pass
74.00	74	74.0	0.0	0.30	1.1	Pass
69.00	69	69.0	0.0	0.30	1.1	Pass
64.00	64	64.0	0.0	0.30	1.1	Pass
59.00	59	59.0	0.0	0.30	1.1	Pass
54.00	54	54.0	0.0	0.30	1.1	Pass
49.00	49	49.0	0.0	0.30	1.1	Pass
44.00	44	44.0	0.0	0.30	1.1	Pass
39.00	39	39.0	0.0	0.30	1.1	Pass
34.00	34	34.0	0.0	0.30	1.1	Pass
29.00	29	29.1	0.1	0.30	1.1	Pass
24.00	24	24.3	0.3	0.30	1.1	Pass

Certificate No : 25-SLM-108
Request No : Req-2025-0595

9. Level linearity including the level range control

UUC Setting	STD	Measured			UNCERTAINTY (\pm dB)	Acceptance Limit (\pm dB)	Result
		REF	UUC	ERR			
FAST / A	(dB)	(dB)	(dB)	(dB)	(\pm dB)	(\pm dB)	
UUC Range	(dB)	(dB)	(dB)	(dB)	(\pm dB)	(\pm dB)	
30-130	29.30	29.5	0.2	0.30	1.1	Pass	
	114	114.0	0.0				

10. Tone burst response

UUC Setting	STD	Anticipated	Measured		UNCERTAINTY (\pm dB)	Acceptance Limit (\pm dB)	Result
			REF	ERR			
FAST / A / 30-130	(ms)	(dB)	(dB)	(dB)	(\pm dB)	(\pm dB)	
UUC Time Response	(ms)	(dB)	(dB)	(dB)	(\pm dB)	(\pm dB)	
Fast	200	126.0	126.0	0.0	0.20	1.0	Pass
	2	109.0	109.0	0.0		+1.0, -2.5	Pass
	0.25	100.0	99.9	-0.1		+1.5, -5.0	Pass
Slow	200	119.6	119.6	0.0	0.20	1.0	Pass
	2	100.0	100.0	0.0		+1.0, -5.0	Pass
	0.25	100.0	100.0	0.0		+1.0, -2.5	Pass
SEL	200	120.0	120.0	0.0	0.20	1.0	Pass
	2	100.0	100.0	0.0		+1.0, -2.5	Pass
	0.25	91.0	90.9	-0.1		+1.5, -5.0	Pass

11. Peak C Sound level

UUC Setting	Anticipated	Measured		UNCERTAINTY (\pm dB)	Acceptance Limit (\pm dB)	Result
		REF	ERR			
FAST / C / 35-141	(dB)	(dB)	(dB)	(\pm dB)	(\pm dB)	
STD Setting	(dB)	(dB)	(dB)	(\pm dB)	(\pm dB)	
Complete cycle	136.4	135.8	-0.60	0.20	3.0	Pass
Positive half cycle	135.4	135.2	-0.20		2.0	Pass
Negative half cycle	135.4	135.2	-0.20		2.0	Pass

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the head of Calibration Laboratory.

เอกสารไม่ควบคุม

FSI-708-SLM-01 Rev.00 Issue date 5/8/24

Certificate No : 25-SLM-108
Request No : Req-2025-0595

12. Overload indication

UUC Setting	Measured	UNCERTAINTY (\pm dB)	Acceptance Limit (\pm dB)	Result
FAST / A / 30-130	UUC			
STD Setting	(dB)	(\pm dB)	(\pm dB)	
Positive one-half cycle	139.4	0.20	1.5	Pass
Negative one-half cycle	139.4			
Deviated	0.0	0.20	1.5	Pass

13. High Level Stability

UUC Setting	Measured	UNCERTAINTY (\pm dB)	Acceptance Limit (\pm dB)	Result
FAST / A / 30-130	UUC			
STD Setting	(dB)	(\pm dB)	(\pm dB)	
Initial	129.0	0.10	0.30	Pass
Final	129.0			
Deviated	0.0	0.10	0.30	Pass

Note :

Function	Maximum-permitted Uncertainty of measurement
1. Indication at the calibration check frequency	Not applicable
2. Self-generated noise. Microphone installed	Not applicable
3. Self-generated noise. Microphone replaced by the electrical input signal device	Not applicable
4. Acoustic signal test of frequency weightings at 10 Hz to 4 kHz	0.60 dB
4. Acoustic signal test of frequency weightings at >4 kHz to 10 kHz	0.70 dB
5. Electrical signal test of frequency weightings. Weighting network response with relative to 1 kHz	0.20 dB
6. Frequency and time weightings at 1 kHz	0.20 dB
7. Long Term Stability	0.10 dB
8. Level linearity on the reference level range	0.30 dB
9. Level linearity including the level range control	0.30 dB
10. Tone burst response	0.30 dB
11. Peak C Sound level	0.25 dB
12. Overload indication	0.25 dB
13. High Level Stability	0.10 dB

* Acceptance limit and Maximum-permitted Uncertainty was REC 61673-1:2011

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the head of Calibration Laboratory.

เอกสารไม่ควบคุม

FSI-708-SLM-01 Rev.00 Issue date 5/8/24

Certificate No : 25-SLM-108
Request No : Req-2025-0595

Decision Rule for Statements of Conformity


The standard decision rule employed for the statements of conformity in each calibration result will be applied using ILAC-G8-09:2019: Guidelines on the Reporting of Compliance with Specification as following Fig. and statements:

Pass - The measurement result plus the expanded uncertainty with a 95% coverage probability were within the limits.

Pass¹ - The measurement result was within the limit. However, a portion of the expanded uncertainty of measurement at 95% exceeds the limit.

Fail¹ - The measurement result was not of the limit. However, a portion of the expanded uncertainty of measurement at 95% is within the limit.

Fail - The measurement result plus the expanded uncertainty with a 95% coverage probability were outside the limits.

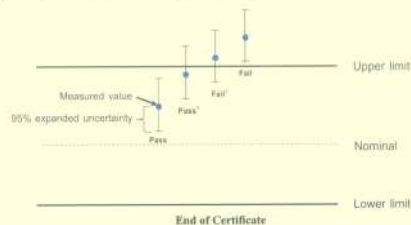

End of Certificate

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the head of Calibration Laboratory.

เอกสารไม่ควบคุม

FSI-708-SLM-01 Rev.00 Issue date 5/8/24

SITHIPORN ASSOCIATES CO., LTD. CALIBRATION LABORATORY

451-451/ Sirinthon Road, Bangsumru, Bangkok, 10700 Thailand
Tel. +66 2433 8331 Email: calibration@sithiporn.com

Cert. No. : ACL25230
Pages : 1 of 8

Calibration Certificate

Equipment : SOUND LEVEL METER
Manufacturer : RION
Model : NL-42 / Microphone UC-52 / Preamplifier NH-24
Serial No.: 00409023 / 185669 / 90468
ID No.: UAEFEM.011/2564

Condition As Found : GOOD

Customer : UNITED ANALYST AND ENGINEERING CONSULTANT (UAE)
81 SOI UDUMSUH 41, SUKHUMVIT ROAD,
BANGCHAK SUB-DISTRICT,
PHRAKHANONG DISTRICT, BANGKOK 10260
THAILAND.

Location : -
Ambient Temperature : (23.0 \pm 3) °C
Pressure : (101.3 \pm 3) kPa
Relative Humidity : (50.0 \pm 20) %

Received Date : 26 MAY 2025
Calibration Date : 10 - 11 JUNE 2025
Date of Issue : 13 JUNE 2025

Calibrated by : Nathakorn Pisutpaisan

Approved by : Wichok E.
(Wichok Ekpongpradit)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

เอกสารไม่ควบคุม

Cert. No. : ACL25230
Job No. : VC68AC0113
Pages : 2 of 8

Calibration Procedure : CP-AC-01

Calibration Method :

This equipment was calibrated by follow on IEC-61672-3 (2013) Standard for sound level meter (SLM).
The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.

For tests results of each items were made by observation of each Instruments display and also with SLM's display.

Condition of this result of calibration :

1. Reference Standard Instruments :

Instrument	Model	Serial No.	Cert. No.	Due Date
Waveform Generator	33210A	MY48017076	EF-0011-25	11-FEB-26
Waveform Generator	33511B	MY52302742	EF-0012-25	11-FEB-26
Digital Multimeter	33461A	MY53220104	EEL-BP 24/0268	22-APR-26
Digital Multimeter	33461A	MY53220076	EEL-BP 23/0268	22-APR-26
Digital Multimeter	34461A	MY60024273	CA2025120EA	18-MAR-26
Programmable Attenuator	MAT-1070	62100114	EF-0006-25	11-FEB-26
Condenser Microphone	4180	2977900	AA-1002-25	19-FEB-26
Measuring Amplifier	NA-42KA1	34560495	AA-3002-25	19-FEB-26

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is traceable to the international system of unit maintained at :

- 3.1 National Institute of Metrology (Thailand).
- 3.2 Thailand Institute of Scientific and Technological Research (TISTR).
- 3.3 Electrical And Electronics Institute (EEI).

เอกสารไม่ควบคุม

michana E.

Cert. No. : ACL25230
Job No. : VC68AC0113
Pages : 3 of 8

Summary of Measurement Result :

Parameter	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	0.2	N/A
2. Self-generated noise	0.2	N/A
3. Acoustical signal tests of frequency weightings		
125 Hz	0.3	0.6
1000 Hz	0.3	0.6
8000 Hz	0.3	0.7
4. Electrical signal tests of frequency weightings		
For 10 Hz to 4 kHz	0.3	0.6
For > 4 kHz to 10 kHz	0.3	0.7
For > 10 kHz to 20 kHz	0.3	1.0
5. Frequency and time weightings at 1 kHz	0.2	0.2
6. Long - term stability	0.1	0.1
7. Level linearity on the reference level range	0.2	0.3
8. Level linearity including the level range control	0.2	0.3
9. Tone burst response	0.2	0.3
10. Peak C sound level	0.2	0.35
11. Overload indication	0.2	0.25
12. High level stability	0.1	0.1

เอกสารไม่ควบคุม

michana E.

Cert. No. : ACL25230
Job No. : VC68AC0113
Page : 4 of 8

Result of calibration :

1. Absolute sensitivity

Reference Acoustic Signal (dB)	Measured Value (dB)	Deviation (dB)	Acceptance Limit (dB)
93.9 (93.94)	93.9	0.0	±0.3

2. Self-generated noise

2.1 Normal test

Measured Value (dB)
15.4

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Weighting (dB)
A - weight	12.6
C - weight	18.5
Flat	24.1

3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency (Hz)	Flat	C-weight	A-weight	Acceptance Limits
125	0.1	0.1	0.1	±1.5
1000	0.1	0.1	0.1	±1.0
8000	2.3	2.4	2.4	±5.0

เอกสารไม่ควบคุม

michana E.

Cert. No. : ACL25230
Job No. : VC68AC0113
Pages : 5 of 8

4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Flat	C-weight	A-weight	Acceptance Limits
63	0.0	-0.1	-0.1	±2.0
125	0.0	0.0	0.0	±1.5
250	0.0	-0.1	-0.1	±1.5
500	0.0	0.0	-0.1	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.0	0.0	±2.0
4000	0.0	0.0	0.0	±3.0
8000	0.0	0.0	0.0	±5.0

5. Frequency and time weightings at 1 kHz

5.1 Frequency weightings at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	±0.2
C - weight	94.0	94.0	0.0	±0.2
Flat	94.0	94.0	0.0	±0.2

5.2 Time weighting at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	94.0	94.0	0.0	±0.1
Slow	94.0	94.0	0.0	±0.1
Leq	94.0	94.0	0.0	±0.1

6. Long - term stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	±0.3

เอกสารไม่ควบคุม

michana E.

Cert. No. : ACL25230
Job No. : VC68AC0113
Pages : 6 of 8

7. Level linearity on the reference level range

Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
137.0	137.0	0.0	± 1.1
136.0	136.1	0.1	± 1.1
135.0	135.1	0.1	± 1.1
134.0	134.1	0.1	± 1.1
133.0	133.0	0.0	± 1.1
132.0	132.0	0.0	± 1.1
131.0	131.0	0.0	± 1.1
129.0	129.1	0.1	± 1.1
124.0	124.0	0.0	± 1.1
119.0	119.1	0.1	± 1.1
114.0	114.1	0.1	± 1.1
109.0	109.1	0.1	± 1.1
104.0	104.1	0.1	± 1.1
99.0	99.1	0.1	± 1.1
94.0	94.0	0.0	± 1.1
89.0	89.0	0.0	± 1.1
84.0	84.0	0.0	± 1.1
79.0	79.0	0.0	± 1.1
74.0	74.0	0.0	± 1.1
69.0	69.0	0.0	± 1.1
64.0	64.0	0.0	± 1.1
59.0	59.0	0.0	± 1.1
54.0	54.0	0.0	± 1.1
49.0	49.0	0.0	± 1.1
44.0	44.0	0.0	± 1.1
39.0	39.0	0.0	± 1.1
34.0	34.0	0.0	± 1.1
30.0	30.0	0.0	± 1.1
29.0	29.0	0.0	± 1.1
28.0	28.0	0.0	± 1.1
27.0	27.0	0.0	± 1.1
26.0	26.0	0.0	± 1.1
25.0	25.0	0.0	± 1.1

เอกสารไม่ควบคุม

prichan B.

Cert. No. : ACL25230
Job No. : VC68AC0113
Pages : 7 of 8

8. Level linearity including the level range control

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
130	94.0	94.0	0.0	±1.1

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
130	29.0	28.9	-0.1	±1.1

9. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Cycle	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	116.9	-0.1	1.0 ; -2.5
	200	800	134.0	134.0	0.0	±1.0
Slow	2	8	108.0	108.0	0.0	1.0 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
SEL	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.0	0.0	±1.0

เอกสารไม่ควบคุม

prichan B.

Cert. No. : ACL25230
Job No. : VC68AC0113
Pages : 8 of 8

10. Peak C sound level

Number of cycle in test signal	Anticipated Value (dB)	Measured Value, L _{peak} (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	130.0	130.0	0.0	±3.0
One	133.4	133.4	0.0	±3.0

Number of cycle in test signal	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	±2.0
Positive half cycle	135.4	135.1	-0.3	±2.0
Negative half cycle	135.4	135.1	-0.3	±2.0

11. Overload indication

Measured value (dB)		Deviated Value (dB)	Acceptance Limits (dB)
Positive one-half cycle	Negative one-half cycle		
89.5	89.5	0.0	±1.5

12. High level stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor $k = 2$ or any value following calculation, providing a level of confidence of approximately 95 %

End of Calibration Certificate

เอกสารไม่ควบคุม

prichan B.