ภาคผนวก จ

หนังสือรับรองการสอบเทียบเครื่องมือ

ภาคผนวก จ-1

บริษัท อินทิเกรทเต็ด รีเซิร์ซ เซ็นเตอร์ จำกัด

JIRANATEE ASSOCIATES CO.,LTD.

Jiranatee Associates Co.,Ltd
63/14-15, 67/35-36
Petchkasem 7,7/1, Rd.Watthapra, Bangkokyai,
Bangkok 10600(Thailand)
Tel: +6608680812
Mobile: +66863999453
E-mail: jnac-calibration@jiranatee.com
Web site: www.jiranatee.com

Accredited calibration laboratory
ISO/IEC 17025:2017
NSC-TISI-TIS 17025
CALIBRATION 0367

Flow measurement laboratory
Calibration services department.

NSC – TISI – TIS 17025
CALIBRATION 0367

CERTIFICATE OF CALIBRATION

Certificate No. : COF-022-68

MEASUREMENT ITEM : Top Load Orifice
MANUFACTURER : TISCH
MODEL/TYPE : TE-5028A
SERIAL NUMBER : 2926
ID NUMBER : -
CONDITION AS-RECEIVED : Used item
CUSTOMER : Integrated Research Center Company Limited.
122 Moo 2, Thatoom, Srimahaphote,
Prachinburi 25140, Thailand.

RECEIVED DATE : 05 Jun 2025
MEASUREMENT DATE : 12 Jun 2025
ISSUE DATE : 13 Jun 2025

ENVIRONMENTAL CONDITIONS:
Ambient condition in the laboratory are as follow:

Temperature	: 23.0 ± 3.0	°C
Relative Humidity	: 55.0 ± 15.0	%RH
Atmospheric Pressure	: 1010 ± 10	hPa

CALIBRATION CONDITION:
Preconditioning : 24 hours at ambient conditions.
Measurement Condition : The average values during measurement are 22.7 °C and 52.1 %RH.

***NOTED:** The certificate is valid only to the item calibrated on date and place of calibration.*

TABULATION OF RESULTS:
The table on next page give the measured values.

Calibration procedure:
The Orifice gas flow device was calibrated against Standard Rotary Displacement Meter (Roots Meter) Model G65/IMC/W2-dp. The WI-CL-004 was used as a calibration guideline.

Traceability:
This certificate provides a traceability of the measurement to recognized the national standards, and to realization of the international system of units (SI) through the NIMT (National Metrology Institute of Thailand) via Certificate number: MW-0016-25.

Uncertainty of Measurement:
The reported uncertainty of measurement is based on the standard uncertainty multiplied by a coverage factor k=2, Which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty has been determined in accordance with the GUM 'Evaluation of measurement data - Guide to the expression of uncertainty in measurement'

Calibrated by:
☐ Mr. Sorawit Thachalad
☑ Miss Jittraporn Lertsomphol

Approved signatory:
Mr. Parinya Booncharoen
Calibration Department Manager

THIS CERTIFICATE OF CALIBRATION MAY NOT BE REPRODUCED EXCEPT IN FULL UNLESS PERMISSION FOR REPRODUCTION HAS BEEN OBTAINED IN WRITING FROM THE LABORATORY

JIRANATEE ASSOCIATES CO.,LTD.

Continuation of Certificate of Calibration Number COF-022-68

MEASUREMENT RESULTS:

The Orifice gas flow device was calibrated by direct comparison method with the Standard Rotary Displacement Meter (Roots Meter). The Humid air was used as a medium in the system. The standard conditions are 25°C (298.15 K) and 760 mmHg for standard temperature and standard pressure respectively.

Table 1: The results of Q Standard calibration data

Plate	Flow rate m^3/min	Pressure [Pa] mmHg	Temperature [Ta] °C	Temperature [Tm] °C	Δp_meter mmHg	Δp_Orifice inH_2O	Y	Standard Flow [Q_s] m^3/min
1	0.698	752.986	22.65	22.05	60.043	1.071	1.034	0.643
2	1.003	752.904	22.57	21.90	44.794	2.326	1.524	0.944
3	1.120	752.767	22.83	22.21	39.589	2.939	1.712	1.061
4	1.167	752.907	22.91	22.32	37.026	3.231	1.795	1.109
5	1.417	752.831	23.13	22.57	25.460	4.930	2.217	1.368

Slope (m): 1.63233
Intercept (b): -0.01636
Correlation coefficient (r): 0.99980
Uncertainty ($k=2$): 0.015 m^3/min

Table 2: The results of Q actual calibration data

Plate	Flow rate m^3/min	Pressure [Pa] mmHg	Temperature [Ta] °C	Temperature [Tm] °C	Δp_meter mmHg	Δp_Orifice inH_2O	Y	Standard Flow [Q_a] m^3/min
1	0.698	752.986	22.65	22.05	60.043	1.071	0.649	0.644
2	1.003	752.904	22.57	21.90	44.794	2.326	0.956	0.945
3	1.120	752.767	22.83	22.21	39.589	2.939	1.075	1.063
4	1.167	752.907	22.91	22.32	37.026	3.231	1.127	1.112
5	1.417	752.831	23.13	22.57	25.460	4.930	1.393	1.372

Slope (m): 1.02238
Intercept (b): -0.01025
Correlation coefficient (r): 0.99981
Uncertainty ($k=2$): 0.015 m^3/min

End of Certificate of Calibration

JIRANATEE ASSOCIATES CO.,LTD.

Jiranatee Associates Co.,Ltd.

DKSH

NSC-TISI-TIS 17025 Calibration 0067

Certificate of Calibration

Equipment:	Electronic Balance	Certificate No.:	C01253238
Manufacturer:	Sartorius	Job No.:	WO-00091491
Model:	BSA224S-CW	Issued Date:	03 November 2025
Serial No.:	34490341	Page:	1 of 2
ID No.:	-		
Condition of the item:	Normal		

Customer: Integrated Research Center Co.,Ltd.
122 Moo 2, Tambol Thatoom,
Amphur Srimahaphote, Prachinburi 25140 Thailand

Environment Condition: Temperature 25 °C ± 0.5 °C
Relative Humidity 67 % ± 3.3 %

Calibration Place: Double A (1991) Public Company Limited.
(Water Labaratory IP1 (Balance Room))
1 Moo 2, Thatoom, Srimahaphot,
Prachinburi 25140 Thailand.

Calibration By: Mr. Piyapat Saidoung

Calibration Date: 28 October 2025

The Method Used: In-house method, CAL-WI-47, based on UKAS Lab 14

Traceability: This certificate is traceable to the SI Units maintained by National Institute of Metrology (NIMT), Thailand through DKSH Technology Co., Ltd. Certificate No. C02250448

(Mr. Piyapat Saidoung)
Person in charge

(Mr. Adisai Maknoi)
Authorized signatory

This certificate is issued the units of measurement according to the International System of Units (SI). It provides traceability of measurement to international or national standard or other recognized national standard laboratories.
The measurement uncertainty stated is the expanded uncertainty which is obtained from the standard uncertainty multiplied by the coverage factor (k=2) to provide a level of confidence of approximately 95%. It is determined in accordance with Evaluation of measurement data - Guide to the expression of uncertainty in measurement (JCGM 100).
These results may be affected by deviations from specified conditions. The results relate only to the items tested, calibrated or sampled. The report shall not be reproduced except in full without approval of DKSH Technology Limited.

บริษัท ดีเคเอสเอช เทคโนโลยี จำกัด
DKSH Technology Limited
2533 ถนนสุขุมวิท แขวงสวนหลวง เขตพระโขนง กรุงเทพมหานคร 10260
2533 Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Phone: +66 2639 7000 Email: info.calibration@dksh.com Website: www.dksh.com/scientific-thailand

DKSH

Calibration Results:

Without Adjustment

Eccentric Error: Weight to be 1/3 or 1/2 of Maximum capacity, taken from the center of the pan as a zero reference.



Nominal Test Value 100 (g)

Reference Points (g)				
A	B	C	D	E
-	0.0001	-0.0002	-0.0001	0.0001

Repeatability: Determination of the standard deviation of weighing balance., Readability 0.0001 (g)

Nominal test value (g)	Standard Deviation
20	0.00005
200	0.00007

Error of indication from nominal or conventional mass value., Readability 0.0001 (g)

Nominal Value (g)	Conventional Mass (g)	Displayed Value (g)	Error of indication (g)	Uncertainty (± g)	k
0.1	0.10000	0.1000	0.0000	0.00012	2.06
0.2	0.20000	0.2000	0.0000	0.00012	2.06
0.5	0.50000	0.5000	0.0000	0.00012	2.06
1	1.00001	1.0000	0.0000	0.00012	2.06
2	2.00002	2.0000	0.0000	0.00012	2.06
5	5.00001	5.0000	0.0000	0.00012	2.06
10	10.00001	10.0000	0.0000	0.00012	2.05
20	20.00001	20.0000	0.0000	0.00012	2.05
50	50.00001	50.0000	0.0000	0.00014	2.03
100	99.99992	100.0000	0.0001	0.00018	2.01
200	199.99992	200.0000	0.0001	0.00030	2.00

The End of Certificate

บริษัท ดีเคเอสเอช เทคโนโลยี จำกัด
DKSH Technology Limited
2533 ถนนสุขุมวิท แขวงสวนหลวง เขตพระโขนง กรุงเทพมหานคร 10260
2533 Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Phone: +66 2639 7000 Email: info.calibration@dksh.com Website: www.dksh.com/scientific-thailand

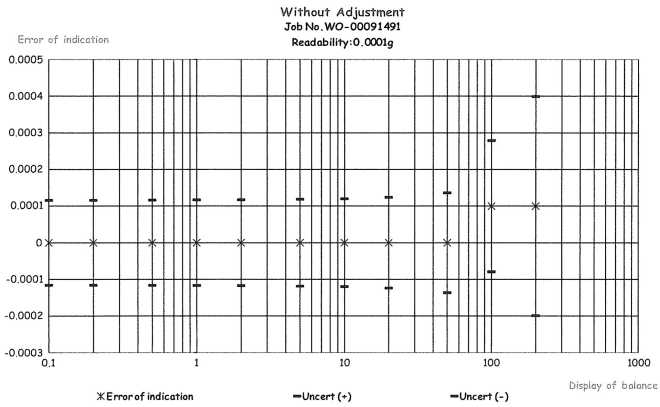

บริษัท ดีเคเอสเอช เทคโนโลยี จำกัด
DKSH Technology Limited
2533 ถนนสุขุมวิท แขวงบางจาก เขตพระโขนง กรุงเทพมหานคร 10260
2533 Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Phone: +66 2639 7000 Email: info.calibration@dksh.com Website: www.dksh.com/scientific-thailand

ใบตรวจสอบสภาพเครื่องชั่ง
Electronic Balance Checklist

Equipment: Electronic Balance
Model: BSA224S-CW
Serial No.: 34490341

Certificate No.: C01253238
Job No.: WO-00091491

Check date 28 Oct 2025 (Normal)	Check date 28 Oct 2025 (Defective)	รายการตรวจเช็ค (Description)	Check before delivery 28 Oct 2025 (Normal)	Check before delivery 28 Oct 2025 (Defective)	หมายเหตุ (Remark)
		General			
☑	☐	1. สายไฟ/ อะแดปเตอร์ (Electrical wire/ Adaptor)	☑	☐	
☑	☐	2. ความสมบูรณ์ชุดกระจกกันลม (Cover)	☑	☐	
☑	☐	3. ความสมบูรณ์ของระดับน้ำ (Bubble spirit level)	☑	☐	
☑	☐	4. ความสมบูรณ์ของชุดขาตั้งเครื่อง (Leveling foot)	☑	☐	
☑	☐	5. การตอบสนองของปุ่มกด (Keys)	☑	☐	
☑	☐	6. ความสมบูรณ์ของหน้าจอ (Display)	☑	☐	
☑	☐	7. การแสดงผลของหน้าจอ (Screen display)	☑	☐	
☑	☐	8. ชุดรองจานชั่ง (Stopper/ Pan support)	☑	☐	
☑	☐	9. การทำงานของฟังค์ชั่น (Internal/ External Function)	☑	☐	
☑	☐	10. ความสะอาดของตัวเครื่องภายนอก (External cleanliness of the balance)	☑	☐	
☑	☐	11. สภาวะแวดล้อม ณ สถานที่ตั้งเครื่องชั่ง (Environment at the location of the balance)	☑	☐	

ข้อแนะนำ/ Note : _____

Mr. Piyapat Saidoung
Service Engineer

บริษัท ดีเคเอสเอช เทคโนโลยี จำกัด
DKSH Technology Limited
2533 ถนนสุขุมวิท แขวงบางจาก เขตพระโขนง กรุงเทพมหานคร 10260
2533 Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Phone: +66 2639 7000 Email: info.calibration@dksh.com Website: www.dksh.com/scientific-thailand

Delivering Growth – in Asia and Beyond.

Certificate of Calibration

NSC-TISI-TIS 17025 Calibration 0067

Equipment: Electronic Balance
Manufacturer: Sartorius
Model: ME36S
Serial No.: 27206085
ID No.: -
Condition of the item: Normal

Certificate No.: C01253246
Job No.: WO-00091493
Issued Date: 03 November 2025
Page: 1 of 2

Customer: Integrated Research Center Co.,Ltd.
122 Moo 2, Tambol Thatoom,
Amphur Srimahaphote, Prachinburi 25140 Thailand

Environment Condition: Temperature 25 °C ± 0.8 °C
Relative Humidity 68 % ± 2.4 %

Calibration Place: Double A (1991) Public Company Limited.
(Water Labaratory IP1 (Balance Room))
1 Moo 2, Thatoom, Srimahaphot,
Prachinburi 25140 Thailand.

Calibration By: Mr. Piyapat Saidoung
Calibration Date: 29 October 2025
The Method Used: In-house method, CAL-WI-47, based on UKAS Lab 14
Traceability: This certificate is traceable to the SI Units maintained by National Institute of Metrology (NIMT), Thailand through DKSH Technology Co., Ltd. Certificate No. C02250448

(Mr. Piyapat Saidoung)
Person in charge

(Mr. Adisai Maknoi)
Authorized signatory

This certificate is issued the units of measurement according to the International System of Units (SI). It provides traceability of measurement to international or national standard or other recognized national standard laboratories.
The measurement uncertainty stated is the expanded uncertainty which is obtained from the standard uncertainty multiplied by the coverage factor (k=2) to provide a level of confidence of approximately 95%. It is determined in accordance with Evaluation of measurement data - Guide to the expression of uncertainty in measurement (JCGM 100).
These results may be affected by deviations from specified conditions. The results relate only to the items tested, calibrated or sampled. The report shall not be reproduced except in full without approval of DKSH Technology Limited.

บริษัท ดีเคเอสเอช เทคโนโลยี จำกัด
DKSH Technology Limited
2533 ถนนสุขุมวิท แขวงบางจาก เขตพระโขนง กรุงเทพมหานคร 10260
2533 Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Phone: +66 2639 7000 Email: info.calibration@dksh.com Website: www.dksh.com/scientific-thailand

Delivering Growth – in Asia and Beyond.

Calibration Results:

Without Adjustment

Eccentric Error: Weight to be 1/3 or 1/2 of Maximum capacity, taken from the center of the pan as a zero reference.



Nominal Test Value 10000 (mg)

Reference Points (mg)				
A	B	C	D	E
-	-0.002	-0.001	0.002	0.001

Repeatability: Determination of the standard deviation of weighing balance., Readability 0.001 (mg)

Nominal test value (mg)	Standard Deviation
2000	0.0007
20000	0.0008

Error of indication from nominal or conventional mass value., Readability 0.001 (mg)

Nominal Value (mg)	Conventional Mass (mg)	Displayed Value (mg)	Error of indication (mg)	Uncertainty (± mg)	k
1	1.0020	1.002	0.000	0.0033	2.00
5	5.0010	5.001	0.000	0.0033	2.00
10	10.0020	10.001	-0.001	0.0040	2.00
50	50.0000	50.000	0.000	0.0063	2.00
100	100.0040	100.003	-0.001	0.0082	2.00
500	500.0030	500.003	0.000	0.013	2.00
1000	1000.0120	1000.012	0.000	0.016	2.00
5000	5000.0120	5000.011	-0.001	0.027	2.00
10000	10000.0100	10000.005	-0.005	0.033	2.00
20000	20000.0070	20000.001	-0.006	0.048	2.00
30000	30000.0170	30000.010	-0.007	0.080	2.00

The End of Certificate

บริษัท ดีเคเอสเอช เทคโนโลยี จำกัด
DKSH Technology Limited
2533 ถนนสุขุมวิท แขวงบางจาก เขตพระโขนง กรุงเทพมหานคร 10260
2533 Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Phone: +66 2639 7000 Email: info.calibration@dksh.com Website: www.dksh.com/scientific-thailand

Delivering Growth – in Asia and Beyond.

CAL-FM-C01-15: 30 Jun 2025

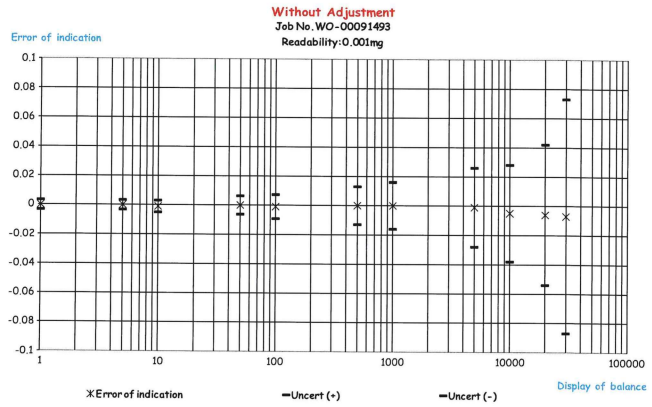

บริษัท ดีเคเอสเอช เทคโนโลยี จำกัด
DKSH Technology Limited
2533 ถนนสุขุมวิท แขวงบางจาก เขตพระโขนง กรุงเทพมหานคร 10260
2533 Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Phone: +66 2639 7000 Email: info.calibration@dksh.com Website: www.dksh.com/scientific-thailand

Delivering Growth – in Asia and Beyond.

ใบตรวจสอบสภาพเครื่องชั่ง
Electronic Balance Checklist

Equipment: Electronic Balance
Model: ME36S
Serial No.: 27206085

Certificate No.: C01253246
Job No.: WO-00091493

Check date 29 Oct 2025 (Normal)	Check date 29 Oct 2025 (Defective)	รายการตรวจเช็ค (Description)	Check before delivery 29 Oct 2025 (Normal)	Check before delivery 29 Oct 2025 (Defective)	หมายเหตุ (Remark)
		General			
☑	☐	1. สายไฟ/ อะแดปเตอร์ (Electrical wire/ Adaptor)	☑	☐	
☑	☐	2. ความสมบูรณ์ชุดกระจกกันลม (Cover)	☑	☐	
☑	☐	3. ความสมบูรณ์ของระดับน้ำ (Bubble spirit level)	☑	☐	
☑	☐	4. ความสมบูรณ์ของชุดขาตั้งเครื่อง (Leveling foot)	☑	☐	
☑	☐	5. การตอบสนองของปุ่มกด (Keys)	☑	☐	
☑	☐	6. ความสมบูรณ์ของหน้าจอ (Display)	☑	☐	
☑	☐	7. การแสดงผลของหน้าจอ (Screen display)	☑	☐	
☑	☐	8. ชุดรองจานชั่ง (Stopper/ Pan support)	☑	☐	
☑	☐	9. การทำงานของฟังค์ชั่น (Internal/ External Function)	☑	☐	
☑	☐	10. ความสะอาดของตัวเครื่องภายนอก (External cleanliness of the balance)	☑	☐	
☑	☐	11. สภาวะแวดล้อม ณ สถานที่ตั้งเครื่องชั่ง (Environment at the location of the balance)	☑	☐	

ข้อแนะนำ/ Note :

Mr. Piyapat Saidoung
Service Engineer

บริษัท ดีเคเอสเอช เทคโนโลยี จำกัด
DKSH Technology Limited
2533 ถนนสุขุมวิท แขวงบางจาก เขตพระโขนง กรุงเทพมหานคร 10260
2533 Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Phone: +66 2639 7000 Email: info.calibration@dksh.com Website: www.dksh.com/scientific-thailand

Delivering Growth – in Asia and Beyond.

THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-68/0159 **MTC No.** EEL. BP. 80/0168

CALIBRATION CERTIFICATE

Submitted by : Integrated Research Center Company Limited.
Address : 122 Moo 2, T.Thatoom, A.Srimahaphote, Pachinburi, 25140.
Calibrated at : Electrical and Electronic Standards Laboratory, Industrial Metrology and Testing Service Centre.
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Rd., Muang, Samutprakan 10280.

Instrument Calibrated :
Description : Sound Calibrator
Manufacturer : ACO
Model : 2127
Serial No. : 100012

Ambient Environment
Temperature : (23 + 3) °C
Relative Humidity : (50 ± 15) %
Ambient Pressure : (101.325 ± 1.500) kPa

Standards used :
1. Digital Function Synthesizer NF Electronic DF-193A S/N 122037.
2. Measuring Amplifier Bruel&Kjaer 2636 S/N 1537484.
3. Programmable Attenuator Tamagawa TPA-303A S/N OF 2214.
4. Digital Multimeter Agilent 34401A S/N MY44005560.
5. Pressure Transmitter Vaisala PTB202AD S/N T0650001.
6. Audio Analyzer Panasonic VP-7722A S/N 041477D122.
7. Condenser Microphone B&K 4180 S/N 2889871.

Calibration Procedure: CP-102-04 based on IEC 60942-2003; The sound pressure level generated by sound calibrator under test shall be measured by standard microphone using an insert voltage technique.

This instrument has been calibrated against standards maintained at Electrical and Electronic Standards Laboratory (EEL), which are traceable to the International System of Units through the National Institute of Metrology (Thailand).

The information on actual reading is attached herewith and the uncertainty limits quoted refer to the measured values only.

Date of Receipt : 14 Jan. 2025
Date of Calibration : 21 Jan. 2025

The results relate only to the items tested/calibrated or value assigned.
Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang, Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9009

Office/Laboratory
668 Mu 2 Tambon Bangpoomai, Amphoe Muang Samutprakan, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtc@tistr.or.th Website : www.tistr.or.th

Office
196 Phahonyothin Road, Ladyao, Chatuchak, Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827

THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-68/0159 **MTC No.** EEL. BP. 80/0168

The reported expanded uncertainty is based upon a standard uncertainty multiplied by a coverage factor k = 2, providing a level of confidence of approximately 95%.

Nominal Output of Unit Under Test = 94 dB re 20µPa at 1000 Hz

Acoustic Output in dB re 20µPa, Corrected to Reference Conditions: 101.325 kPa, 23.0 °C and 50 %RH.

1. Sound Pressure Level

Standard Microphone Type	Measured Sound Pressure Level (dB)	Deviated value (dB)	Uncertainty (dB)	Tolerance limit IEC60942:2003 Class 1
1/2 inch Bruel&Kjaer 4180	93.91	-0.09	± 0.10	±0.40 dB

2. Frequency

Standard Microphone Type	Measured Frequency (Hz)	Deviated value (Hz)	Uncertainty (Hz)	Tolerance limit IEC60942:2003 Class 1
1/2 inch Bruel&Kjaer 4180	1000.0	0.0	± 1.5	±1.0%

3. Total Distortion

Standard Microphone Type	Measured Total Distortion (%)	Uncertainty (%)	Tolerance limit IEC60942:2003 Class 1
1/2 inch Bruel&Kjaer 4180	1.50	± 0.50	±3.0%

Note : 1. No adjustment.
2. The calibrator pressure correction was not included.
3. The microphone volume correction was not included.

Calibrated by : (Mr.Weerachai Deechaiyae)

Approved by : (Mr.Prawate Kluaypa)
Director
Electrical and Electronic Standards Laboratory
Industrial Metrology and Testing Service Centre

Date of Calibration : 21 Jan. 2025
Date of Issue : 23 Jan. 2025
Ref : 2011268011400184001

End of Certificate

The results relate only to the items tested/calibrated or value assigned.
Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.5

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang, Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9009

Office/Laboratory
668 Mu 2 Tambon Bangpoomai, Amphoe Muang Samutprakan, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtc@tistr.or.th Website : www.tistr.or.th

Office
196 Phahonyothin Road, Ladyao, Chatuchak, Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827

THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-68/0160 **MTC No.** EEL. BP. 94/0168

CALIBRATION CERTIFICATE

Submitted by : Integrated Research Center Company Limited.

Address : 122 Moo 2, T.Thatoom, A.Srimahaphote, Prachinburi, 25140.

Calibrated at : Electrical and Electronic Standards Laboratory, Industrial Metrology and Testing Service Centre.
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Rd., A.Muang, Samutprakan 10280.

Instrument Calibrated :

Description	: Sound Level Meter
Manufacturer	: Delta OHM
Model	: HD 2010UC
Serial No.	: 11040842479
Microphone	: Type UC-52 No.114674
Preamplifier	: Delta Type HD2010PNE2 No.11001018

Ambient Environment

Temperature	: (23 ± 3) °C
Relative Humidity	: (50 ± 15) %
Ambient Pressure	: (101.325±1.5) kPa

Standards used :

1. Band Pass Filter Stanford Research Systems SR 650 S/N 28712.
2. Condenser Microphone Brüel&Kjær 4180 S/N 2889871.
3. Decade Attenuator Ando AL-205 S/N 00464602.
4. Function/Arbitrary Waveform Generator Agilent 33220A S/N MY44042668.
5. Digital Function Synthesizer NF Electronic Instruments DF-193A S/N 122037.
6. Sound Calibrator Bruel&Kjaer 4231 S/N 3015154.
7. Measuring Amplifier Brüel&Kjær 2636 S/N 1537484.

Date of Receipt : 14 Jan. 2025

Date of Calibration : 17-18 Feb. 2025

The results relate only to the items tested/calibrated or value assigned.
Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang, Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9009

Office/Laboratory
668 Mu 2 Tambon Bangpoomai, Amphoe Muang Samutprakan, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtc@tistr.or.th Website : www.tistr.or.th

Office
196 Phahonyothin Road, Ladyao, Chatuchak, Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827

NSC-TISI-TIS 17025
CALIBRATION 0037

THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-68/0160 **MTC No.** EEL. BP. 94/0168

8. Power Amplifier Brüel&Kjær 2706 S/N 1517650.
9. Speaker Tannoy Limited, Great Britain British Patent No. 215300.
10. Digital Multimeter Agilent 34401A S/N MY44005560.
11. Programmable Attenuator Tamagawa TPA-303A S/N 2212.

Calibration Procedure :

This instrument was calibrated by using calibration procedures no CP-102-02 and CP-102-03, which were based on IEC 61672-3 Electroacoustics - Sound Level Meters - Part 3 : Periodic tests (2013). These calibration procedures were related to the electrical and acoustic signal tests. The electrical signal test was carried out with the direct measurement method. The acoustic signal test was performed in an anechoic room with the comparison measurement method.

This instrument has been calibrated against standards maintained at the Electrical and Electronic Standards Laboratory (EEL), which are traceable to the International System of Units through the National Institute of Metrology (Thailand).

The information on actual reading is attached herewith and the uncertainty limits quoted refer to the measured values only.

The reported expanded uncertainty is based upon a standard uncertainty multiplied by a coverage factor k=2, providing a level of confidence of approximately 95%.

Date of Calibration : 17-18 Feb. 2025

The results relate only to the items tested/calibrated or value assigned.
Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.5

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang, Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9009

Office/Laboratory
668 Mu 2 Tambon Bangpoomai, Amphoe Muang Samutprakan, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtc@tistr.or.th Website : www.tistr.or.th

Office
196 Phahonyothin Road, Ladyao, Chatuchak, Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827

NSC-TISI-TIS 17025
CALIBRATION 0037

THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-68/0160 **MTC No.** EEL. BP. 94/0168

1. Absolute Sensitivity

Reference Acoustic Signal (dB)	Measured value (dB)		Deviation value (dB)	Acceptance limit Class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
	Before adjust	After adjust				
93.95	93.3	94.0	0.1	1.0	0.30	N/A

Note: The external calibration adjustment was firstly performed. The internal calibration adjustment was then completed at the display of 94.0 dB.

2. Self-generated noise

2.1 Normal test

Measured value (dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
19.6	0.10	N/A

2.2 The microphone of the sound level meter was replaced by electrical signal input device

Frequency Weighting	Measured value (dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
A-Weight	18.3	0.10	N/A
C-Weight	24.5	0.20	N/A
Flat	26.9	0.30	N/A

Date of Calibration : 17-18 Feb. 2025

The results relate only to the items tested/calibrated or value assigned.
Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.5

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang, Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9009

Office/Laboratory
668 Mu 2 Tambon Bangpoomai, Amphoe Muang Samutprakan, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtc@tistr.or.th Website : www.tistr.or.th

Office
196 Phahonyothin Road, Ladyao, Chatuchak, Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827

NSC-TISI-TIS 17025
CALIBRATION 0037

THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-68/0160 **MTC No.** EEL. BP. 94/0168

3. Acoustical signal test of frequency weightings

Frequency (Hz)	Deviation from frequency response (dB)			Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
	A-weight	C-weight	Flat			
125	0.4	0.3	0.2	1.5	0.45	0.6
1 000	-0.5	-0.5	-0.5	1.0	0.45	0.6
8 000	-4.0	-3.9	-4.0	5.0	0.45	0.7

4. Electrical signal test of frequency weightings

Frequency (Hz)	Deviation from frequency response (dB)			Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
	A-weight	C-weight	Flat			
63	-0.1	-0.2	-0.3	2.0	0.20	0.6
125	-0.1	-0.1	-0.2	1.5	0.20	0.6
250	0.0	-0.1	-0.1	1.5	0.20	0.6
500	0.0	0.0	0.0	1.5	0.20	0.6
1 000	0.0	0.0	0.0	1.0	0.20	0.6
2 000	0.0	0.1	0.1	2.0	0.20	0.6
4 000	0.1	0.1	0.1	3.0	0.20	0.6
8 000	0.1	0.1	0.1	5.0	0.20	0.7

Date of Calibration : 17-18 Feb. 2025

The results relate only to the items tested/calibrated or value assigned.
Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.5

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang, Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9009

Office/Laboratory
668 Mu 2 Tambon Bangpoomai, Amphoe Muang Samutprakan, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtc@tistr.or.th Website : www.tistr.or.th

Office
196 Phahonyothin Road, Ladyao, Chatuchak, Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827

THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-68/0160 **MTC No.** EEL. BP. 94/0168

5. Long-term stability

Time	Measured Value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Begin	94.0	0.0	0.3	0.10	0.1
End	94.0				

6. Frequency and time weightings at 1 kHz

6.1 Frequency weightings at 1 kHz

Frequency Weighting	Measured Value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
A-weight	94.0	0.0	0.2	0.20	0.2
C-weight	94.0	0.0	0.2	0.20	0.2
Flat	94.1	0.1	0.2	0.20	0.2

6.2 Time weightings at 1 kHz

Frequency Weighting	Measured Value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Fast	94.0	0.0	0.1	0.20	0.2
Slow	94.0	0.0	0.1	0.20	0.2
Leq	94.0	0.0	0.1	0.20	0.2

Date of Calibration : 17-18 Feb. 2025

The results relate only to the items tested/calibrated or value assigned.
Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang, Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9009

Office/Laboratory
668 Mu 2 Tambon Bangpoomai, Amphoe Muang Samutprakan, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtc@tistr.or.th Website : www.tistr.or.th

Office
196 Phahonyothin Road, Ladyao, Chatuchak, Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827

NSC-TISI-TIS 17025
CALIBRATION 0037

THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-68/0160 **MTC No.** EEL. BP. 94/0168

7. Level linearity on the reference level range

Anticipated value (dB)	Measured Value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
120	120.0	0.0	1.1	0.30	0.3
119	119.0	0.0	1.1	0.30	0.3
114	114.0	0.0	1.1	0.30	0.3
109	109.0	0.0	1.1	0.30	0.3
104	104.0	0.0	1.1	0.30	0.3
99	99.0	0.0	1.1	0.30	0.3
94	94.0	0.0	1.1	0.30	0.3
89	89.0	0.0	1.1	0.30	0.3
84	84.0	0.0	1.1	0.30	0.3
79	79.0	0.0	1.1	0.30	0.3
74	74.0	0.0	1.1	0.30	0.3
69	69.0	0.0	1.1	0.30	0.3
64	64.0	0.0	1.1	0.30	0.3
59	59.0	0.0	1.1	0.30	0.3
54	54.0	0.0	1.1	0.30	0.3
49	49.0	0.0	1.1	0.30	0.3
44	44.0	0.0	1.1	0.30	0.3
43	43.0	0.0	1.1	0.30	0.3
42	42.1	0.1	1.1	0.30	0.3

Date of Calibration : 17-18 Feb. 2025

The results relate only to the items tested/calibrated or value assigned.
Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang, Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9009

Office/Laboratory
668 Mu 2 Tambon Bangpoomai, Amphoe Muang Samutprakan, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtc@tistr.or.th Website : www.tistr.or.th

Office
196 Phahonyothin Road, Ladyao, Chatuchak, Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827

NSC-TISI-TIS 17025
CALIBRATION 0037

THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-68/0160 **MTC No.** EEL. BP. 94/0168

7. Level linearity on the reference level range

Anticipated value (dB)	Measured Value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
41	41.1	0.1	1.1	0.30	0.3
40	40.1	0.1	1.1	0.30	0.3
39	39.1	0.1	1.1	0.30	0.3

8. Level linearlity including the level range control

At reference sound level on the reference level range

Range	Anticipated value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
60-140	94.0	94.0	0.0	1.1	0.30	0.3
50-130	94.0	94.0	0.0	1.1	0.30	0.3
40-120	94.0	94.0	0.0	1.1	0.30	0.3
30-110	94.0	94.0	0.0	1.1	0.30	0.3
20-100	94.0	94.0	0.0	1.1	0.30	0.3

Date of Calibration : 17-18 Feb. 2025

The results relate only to the items tested/calibrated or value assigned.
Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang, Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9009

Office/Laboratory
668 Mu 2 Tambon Bangpoomai, Amphoe Muang Samutprakan, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtc@tistr.or.th Website : www.tistr.or.th

Office
196 Phahonyothin Road, Ladyao, Chatuchak, Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827

NSC-TISI-TIS 17025
CALIBRATION 0037

THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-68/0160 **MTC No.** EEL. BP. 94/0168

8. Level linearlity including the level range control

At reference level at 5 dB greater than the under-range on a level range

Range	Anticipated value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
60-140	65	65.0	0.0	1.1	0.30	0.3
50-130	55	55.0	0.0	1.1	0.30	0.3
40-120	45	45.0	0.0	1.1	0.30	0.3
30-110	35	35.2	0.2	1.1	0.30	0.3
20-100	25	25.3	0.3	1.1	0.30	0.3

9. Tone burst response

Time Weighting	Toneburst Duration, Tb (ms)	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Fast	200	115.8	-0.2	±1.0	0.20	0.3
	2	98.8	-0.2	+1.0; -2.5	0.20	0.3
	0.25	89.6	-0.4	+1.5; -5.0	0.20	0.3
Slow	200	109.4	-0.2	±1.0	0.20	0.3
	2	89.8	-0.2	+1.0; -5.0	0.20	0.3
SEL	200	109.9	-0.1	±1.0	0.20	0.3
	2	90.0	0.0	+1.0; -2.5	0.20	0.3
	0.25	80.9	-0.1	+1.5; -5.0	0.20	0.3

Date of Calibration : 17-18 Feb. 2025

The results relate only to the items tested/calibrated or value assigned.
Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang, Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9009

Office/Laboratory
668 Mu 2 Tambon Bangpoomai, Amphoe Muang Samutprakan, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtc@tistr.or.th Website : www.tistr.or.th

Office
196 Phahonyothin Road, Ladyao, Chatuchak, Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827

THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-68/0160 **MTC No.** EEL. BP. 94/0168

10. Peak C sound level

Number of cycles in test signal	Anticipated value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Complete cycle	135.4	135.3	-0.1	3.0	0.20	0.35
Positive half cycle	134.4	134.2	-0.2	2.0	0.20	0.35
Negative half cycle	134.4	134.2	-0.2	2.0	0.20	0.35

11. Overload indication

Measured value (dB)		Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Positive one-half cycle	Negative one-half cycle				
140.5	140.5	0.0	1.5	0.20	0.25

12. High-level stability

Time	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Begin	139.0	0.0	0.3	0.10	0.1
End	139.0				

Calibrated by : (Mr. Pannasit Phasingsri)

Approved by : (Mr. Prawate Kluaypa)
Director
Electrical and Electronic Standards Laboratory
Industrial Metrology and Testing Service Centre

Date of Calibration : 17-18 Feb. 2025
Date of Issue : 24 Feb. 2025
Ref : 2011268011400185012

End of Certificate

The results relate only to the items tested/calibrated or value assigned.
Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang, Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9009

Office/Laboratory
668 Mu 2 Tambon Bangpoomai, Amphoe Muang Samutprakan, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtc@tistr.or.th Website : www.tistr.or.th

Office
196 Phahonyothin Road, Ladyao, Chatuchak, Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827

NSC-TISI-TIS 17025
CALIBRATION 0037

THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-68/0160 **MTC No.** EEL. BP. 86/0168

CALIBRATION CERTIFICATE

Submitted by : Integrated Research Center Company Limited.
Address : 122 Moo 2, T.Thatoom, A.Srimahaphote, Prachinburi 25140.
Calibrated at : Electrical and Electronic Standards Laboratory, Industrial Metrology and Testing Service Centre.
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Rd., A.Muang, Samutprakan 10280.

Instrument Calibrated :
Description : Sound Level Meter
Manufacturer : ACO
Model : 6236
Serial No. : 212014
Microphone : 7052NR No.76235
Preamplifier : -

Ambient Environment
Temperature : (23 ± 3) °C
Relative Humidity : (50 ± 15) %
Ambient Pressure : (101.325±1.5) kPa

Standards used :

1. Band Pass Filter Stanford Research Systems SR 650 S/N 28712.
2. Condenser Microphone Brüel&Kjær 4180 S/N 2889871.
3. Decade Attenuator Ando AL-205 S/N 00464602.
4. Function/Arbitrary Waveform Generator Agilent 33220A S/N MY44042668.
5. Digital Function Synthesizer NF Electronic Instruments DF-193A S/N 122037.
6. Sound Calibrator Brüel&Kjær 4231 S/N 3015154.
7. Measuring Amplifier Brüel&Kjær 2636 S/N 1537484.

Date of Receipt : 14 Jan.2025
Date of Calibration : 24-27 Feb.2025

The results relate only to the items tested/calibrated or value assigned.
Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang, Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9009

Office/Laboratory
668 Mu 2 Tambon Bangpoomai, Amphoe Muang Samutprakan, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtc@tistr.or.th Website : www.tistr.or.th

Office
196 Phahonyothin Road, Ladyao, Chatuchak, Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827

NSC-TISI-TIS 17025
CALIBRATION 0037

THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-68/0160 **MTC No.** EEL. BP. 86/0168

8. Power Amplifier Brüel&Kjær 2706 S/N 1517650.
9. Speaker Tannoy Limited, Great Britain British Patent No. 215300.
10. Digital Multimeter Agilent 34401A S/N MY44005560.
11. Programmable Attenuator Tamagawa TPA-303A S/N 2212.

Calibration Procedure :

This instrument was calibrated by using calibration procedures no CP-102-02 and CP-102-03, which were based on IEC 61672-3 Electroacoustics - Sound Level Meters - Part 3 : Periodic tests (2013). These calibration procedures were related to the electrical and acoustic signal tests. The electrical signal test was carried out with the direct measurement method. The acoustic signal test was performed in an anechoic room with the comparison measurement method.

This instrument has been calibrated against standards maintained at the Electrical and Electronic Standards Laboratory (EEL), which are traceable to the International System of Units through the National Institute of Metrology (Thailand).

The information on actual reading is attached herewith and the uncertainty limits quoted refer to the measured values only.

The reported expanded uncertainty is based upon a standard uncertainty multiplied by a coverage factor k=2, providing a level of confidence of approximately 95%.

Date of Calibration : 24-27 Feb.2025

The results relate only to the items tested/calibrated or value assigned.
Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang, Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9009

Office/Laboratory
668 Mu 2 Tambon Bangpoomai, Amphoe Muang Samutprakan, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtc@tistr.or.th Website : www.tistr.or.th

Office
196 Phahonyothin Road, Ladyao, Chatuchak, Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827

NSC-TISI-TIS 17025
CALIBRATION 0037

THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-68/0160 **MTC No.** EEL. BP. 86/0168

1. Absolute Sensitivity

Reference Acoustic Signal (dB)	Measured value (dB)		Deviation value (dB)	Acceptance limit Class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (+dB)
	Before adjust	After adjust				
93.99	94.2	94.0	0.0	1.0	0.48	N/A

Note: The external calibration adjustment was firstly performed. The internal calibration adjustment was then completed at the display of 114.7 dB.

2. Self-generated noise

2.1 Normal test

Measured value (dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
20.7	0.10	N/A

2.2 The microphone of the sound level meter was replaced by electrical signal input device

Frequency Weighting	Measured value (dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
A-Weight	13.7	0.10	N/A
C-Weight	19.0	0.10	N/A
Flat	23.9	0.10	N/A

Date of Calibration : 24-27 Feb.2025

The results relate only to the items tested/calibrated or value assigned.
Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang, Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9009

Office/Laboratory
668 Mu 2 Tambon Bangpoomai, Amphoe Muang Samutprakan, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtc@tistr.or.th Website : www.tistr.or.th

Office
196 Phahonyothin Road, Ladyao, Chatuchak, Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827

THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-68/0160 **MTC No.** EEL. BP. 86/0168

3. Acoustical signal test of frequency weightings

Frequency (Hz)	Deviation from frequency response (dB)			Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
	A-weight	C-weight	Flat			
125	0.5	0.5	0.3	1.5	0.45	0.6
1 000	-0.1	-0.2	0.0	1.0	0.45	0.6
8 000	-1.3	-1.1	-0.8	5.0	0.45	0.7

4. Electrical signal test of frequency weightings

Frequency (Hz)	Deviation from frequency response (dB)			Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
	A-weight	C-weight	Flat			
63	0.2	0.0	-0.1	2.0	0.20	0.6
125	0.1	0.0	0.0	1.5	0.20	0.6
250	0.1	0.0	0.0	1.5	0.20	0.6
500	0.0	0.0	0.0	1.5	0.20	0.6
1 000	0.0	0.0	0.0	1.0	0.20	0.6
2 000	-0.1	0.0	-0.1	2.0	0.20	0.6
4 000	-0.4	-0.3	-0.1	3.0	0.20	0.6
8 000	-0.6	-0.6	-0.2	5.0	0.20	0.7

Date of Calibration : 24-27 Feb.2025 4 / 9

The results relate only to the items tested/calibrated or value assigned.
Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang, Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9009

Office/Laboratory
668 Mu 2 Tambon Bangpoomai, Amphoe Muang Samutprakan, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtc@tistr.or.th Website : www.tistr.or.th

Office
196 Phahonyothin Road, Ladyao, Chatuchak, Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827

NSC-TISI-TIS 17025
CALIBRATION 0037

THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-68/0160 **MTC No.** EEL. BP. 86/0168

5. Long-term stability

Time	Measured Value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Begin	94.0	0.0	0.3	0.10	0.1
End	94.0				

6. Frequency and time weightings at 1 kHz

6.1 Frequency weightings at 1 kHz

Frequency Weighting	Measured Value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
A-weight	94.0	0.0	0.2	0.20	0.2
C-weight	94.0	0.0	0.2	0.20	0.2
Flat	94.0	0.0	0.2	0.20	0.2

6.2 Time weightings at 1 kHz

Frequency Weighting	Measured Value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Fast	94.0	0.0	0.1	0.20	0.2
Slow	94.0	0.0	0.1	0.20	0.2
Leq	94.0	0.0	0.1	0.20	0.2

Date of Calibration : 24-27 Feb.2025 5 / 9

The results relate only to the items tested/calibrated or value assigned.
Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.5

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang, Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9009

Office/Laboratory
668 Mu 2 Tambon Bangpoomai, Amphoe Muang Samutprakan, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtc@tistr.or.th Website : www.tistr.or.th

Office
196 Phahonyothin Road, Ladyao, Chatuchak, Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827

NSC-TISI-TIS 17025
CALIBRATION 0037

THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-68/0160 **MTC No.** EEL. BP. 86/0168

7. Level linearity on the reference level range

Anticipated value (dB)	Measured Value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
122	122.1	0.1	1.1	0.30	0.3
121	121.1	0.1	1.1	0.30	0.3
120	120.1	0.1	1.1	0.30	0.3
119	119.1	0.1	1.1	0.30	0.3
114	114.0	0.0	1.1	0.30	0.3
109	109.0	0.0	1.1	0.30	0.3
104	104.0	0.0	1.1	0.30	0.3
99	99.0	0.0	1.1	0.30	0.3
94	94.0	0.0	1.1	0.30	0.3
89	89.0	0.0	1.1	0.30	0.3
84	84.0	0.0	1.1	0.30	0.3
79	79.0	0.0	1.1	0.30	0.3
74	74.1	0.1	1.1	0.30	0.3
69	69.1	0.1	1.1	0.30	0.3
64	64.0	0.0	1.1	0.30	0.3
59	59.0	0.0	1.1	0.30	0.3
54	54.0	0.0	1.1	0.30	0.3
49	49.0	0.0	1.1	0.30	0.3
44	44.0	0.0	1.1	0.30	0.3
39	39.0	0.0	1.1	0.30	0.3
34	34.1	0.1	1.1	0.30	0.3
33	33.2	0.2	1.1	0.30	0.3

Date of Calibration : 24-27 Feb.2025 6 / 9

The results relate only to the items tested/calibrated or value assigned.
Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.5

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang, Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9009

Office/Laboratory
668 Mu 2 Tambon Bangpoomai, Amphoe Muang Samutprakan, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtc@tistr.or.th Website : www.tistr.or.th

Office
196 Phahonyothin Road, Ladyao, Chatuchak, Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827

NSC-TISI-TIS 17025
CALIBRATION 0037

THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-68/0160 **MTC No.** EEL. BP. 86/0168

7. Level linearity on the reference level range

Anticipated value (dB)	Measured Value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
32	32.2	0.2	1.1	0.30	0.3
31	31.3	0.3	1.1	0.30	0.3
30	30.3	0.3	1.1	0.30	0.3

8. Level linearlity including the level range control

At reference sound level on the reference level range

Range	Anticipated value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
40-130	94.0	94.0	0.0	1.1	0.30	0.3
30-120	94.0	94.0	0.0	1.1	0.30	0.3
20-110	94.0	94.0	0.0	1.1	0.30	0.3
20-100	94.0	94.0	0.0	1.1	0.30	0.3

Date of Calibration : 24-27 Feb.2025 7 / 9

The results relate only to the items tested/calibrated or value assigned.
Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.5

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang, Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9009

Office/Laboratory
668 Mu 2 Tambon Bangpoomai, Amphoe Muang Samutprakan, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtc@tistr.or.th Website : www.tistr.or.th

Office
196 Phahonyothin Road, Ladyao, Chatuchak, Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827

THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-68/0160 **MTC No.** EEL. BP. 86/0168

8. Level linearlity including the level range control

At reference level at 5 dB greater than the under-range on a level range

Range	Anticipated value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
40-130	45.0	45.0	0.0	1.1	0.30	0.3
30-120	35.0	35.0	0.0	1.1	0.30	0.3
20-110	25.0	25.3	0.3	1.1	0.30	0.3
20-100	25.0	25.3	0.3	1.1	0.30	0.3
20-90	25.0	25.2	0.2	1.1	0.30	0.3
20-80	25.0	25.2	0.2	1.1	0.30	0.3

9. Tone burst response

Time Weighting	Toneburst Duration, Tb (ms)	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Fast	200	115.8	-0.2	±1.0	0.20	0.3
	2	98.7	-0.3	+1.0; -2.5	0.20	0.3
	0.25	89.2	-0.8	+1.5; -5.0	0.20	0.3
Slow	200	109.5	-0.1	±1.0	0.20	0.3
	2	89.8	-0.2	+1.0; -5.0	0.20	0.3
SEL	200	109.9	-0.1	±1.0	0.20	0.3
	2	89.9	-0.1	+1.0; -2.5	0.20	0.3
	0.25	80.9	-0.1	+1.5; -5.0	0.20	0.3

Date of Calibration : 24-27 Feb.2025

The results relate only to the items tested/calibrated or value assigned.
Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang, Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9009

Office/Laboratory
668 Mu 2 Tambon Bangpoomai, Amphoe Muang Samutprakan, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtc@tistr.or.th Website : www.tistr.or.th

Office
196 Phahonyothin Road, Ladyao, Chatuchak, Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827

NSC-TISI-TIS 17025
CALIBRATION 0037

THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-68/0160 **MTC No.** EEL. BP. 86/0168

10. Peak C sound level

Number of cycles in test signal	Anticipated value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Complete cycle	125.4	125.0	-0.4	3.0	0.20	0.35
Positive half cycle	124.4	124.3	-0.1	2.0	0.20	0.35
Negative half cycle	124.4	124.3	-0.1	2.0	0.20	0.35

11. Overload indication

Measured value (dB)		Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Positive one-half cycle	Negative one-half cycle				
132.5	132.5	0.0	1.5	0.20	0.25

12. High-level stability

Time	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Begin	129.0	0.0	0.3	0.10	0.1
End	129.0				

Calibrated by :

(Mr. Tawikiat Iamsamran)

Approved by :

(Mr. Prawate Kluaypa)
Director
Electrical and Electronic Standards Laboratory
Industrial Metrology and Testing Service Centre

Date of Calibration : 24-27 Feb.2025

Date of Issue : 28 Feb.2025

Ref : 20112680114001850004

End of Certificate

The results relate only to the items tested/calibrated or value assigned.
Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang, Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9009

Office/Laboratory
668 Mu 2 Tambon Bangpoomai, Amphoe Muang Samutprakan, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtc@tistr.or.th Website : www.tistr.or.th

Office
196 Phahonyothin Road, Ladyao, Chatuchak, Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827

NSC-TISI-TIS 17025
CALIBRATION 0037

THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-68/0160 **MTC No.** EEL. BP. 87/0168

CALIBRATION CERTIFICATE

Submitted by : Integrated Research Center Company Limited.

Address : 122 Moo 2, T.Thatoom, A.Srimahaphote, Prachinburi 25140.

Calibrated at : Electrical and Electronic Standards Laboratory, Industrial Metrology and Testing Service Centre.

Soi 1C, Bangpoo Industrial Estate, Sukhumvit Rd., A.Muang, Samutprakan 10280.

Instrument Calibrated :

Description : Sound Level Meter
Manufacturer : ACO
Model : 6236
Serial No. : 212015
Microphone : 7052NR No.76236
Preamplifier : -

Ambient Environment

Temperature : (23 ± 3) °C
Relative Humidity : (50 ± 15) %
Ambient Pressure : (101.325±1.5) kPa

Standards used :

1. Band Pass Filter Stanford Research Systems SR 650 S/N 28712.
2. Condenser Microphone Brüel&Kjær 4180 S/N 2889871.
3. Decade Attenuator Ando AL-205 S/N 00464602.
4. Function/Arbitrary Waveform Generator Agilent 33220A S/N MY44042668.
5. Digital Function Synthesizer NF Electronic Instruments DF-193A S/N 122037.
6. Sound Calibrator Brüel&Kjær 4231 S/N 3015154.
7. Measuring Amplifier Brüel&Kjær 2636 S/N 1537484.

Date of Receipt : 14 Jan.2025

Date of Calibration : 24-27 Feb.2025

The results relate only to the items tested/calibrated or value assigned.
Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang, Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9009

Office/Laboratory
668 Mu 2 Tambon Bangpoomai, Amphoe Muang Samutprakan, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtc@tistr.or.th Website : www.tistr.or.th

Office
196 Phahonyothin Road, Ladyao, Chatuchak, Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827

NSC-TISI-TIS 17025
CALIBRATION 0037

THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-68/0160 **MTC No.** EEL. BP. 87/0168

8. Power Amplifier Brüel&Kjær 2706 S/N 1517650.
9. Speaker Tannoy Limited, Great Britain British Patent No. 215300.
10. Digital Multimeter Agilent 34401A S/N MY44005560.
11. Programmable Attenuator Tamagawa TPA-303A S/N 2212.

Calibration Procedure :

This instrument was calibrated by using calibration procedures no CP-102-02 and CP-102-03, which were based on IEC 61672-3 Electroacoustics - Sound Level Meters - Part 3 : Periodic tests (2013). These calibration procedures were related to the electrical and acoustic signal tests. The electrical signal test was carried out with the direct measurement method. The acoustic signal test was performed in an anechoic room with the comparison measurement method.

This instrument has been calibrated against standards maintained at the Electrical and Electronic Standards Laboratory (EEL), which are traceable to the International System of Units through the National Institute of Metrology (Thailand).

The information on actual reading is attached herewith and the uncertainty limits quoted refer to the measured values only.

The reported expanded uncertainty is based upon a standard uncertainty multiplied by a coverage factor k=2, providing a level of confidence of approximately 95%.

Date of Calibration : 24-27 Feb.2025

The results relate only to the items tested/calibrated or value assigned.
Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang, Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9009

Office/Laboratory
668 Mu 2 Tambon Bangpoomai, Amphoe Muang Samutprakan, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtc@tistr.or.th Website : www.tistr.or.th

Office
196 Phahonyothin Road, Ladyao, Chatuchak, Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827

THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-68/0160 **MTC No.** EEL. BP. 87/0168

1. Absolute Sensitivity

Reference Acoustic Signal (dB)	Measured value (dB)		Deviation value (dB)	Acceptance limit Class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (+dB)
	Before adjust	After adjust				
93.99	94.4	94.0	0.0	1.0	0.48	N/A

Note: The external calibration adjustment was firstly performed. The internal calibration adjustment was then completed at the display of 115.0 dB.

2. Self-generated noise

2.1 Normal test

Measured value (dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
20.7	0.10	N/A

2.2 The microphone of the sound level meter was replaced by electrical signal input device

Frequency Weighting	Measured value (dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
A-Weight	15.1	0.10	N/A
C-Weight	19.9	0.10	N/A
Flat	24.7	0.10	N/A

Date of Calibration : 24-27 Feb.2025

The results relate only to the items tested/calibrated or value assigned.
Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang, Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9009

Office/Laboratory
668 Mu 2 Tambon Bangpoomai, Amphoe Muang Samutprakan, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtc@tistr.or.th Website : www.tistr.or.th

Office
196 Phahonyothin Road, Ladyao, Chatuchak, Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827

NSC-TISI-TIS 17025
CALIBRATION 0037

THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-68/0160 **MTC No.** EEL. BP. 87/0168

3. Acoustical signal test of frequency weightings

Frequency (Hz)	Deviation from frequency response (dB)			Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
	A-weight	C-weight	Flat			
125	0.4	0.6	0.4	1.5	0.45	0.6
1 000	-0.1	-0.1	0.1	1.0	0.45	0.6
8 000	-0.7	-0.7	-0.2	5.0	0.45	0.7

4. Electrical signal test of frequency weightings

Frequency (Hz)	Deviation from frequency response (dB)			Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
	A-weight	C-weight	Flat			
63	0.0	0.0	-0.1	2.0	0.20	0.6
125	-0.1	0.0	0.0	1.5	0.20	0.6
250	0.0	0.0	0.0	1.5	0.20	0.6
500	0.0	0.0	0.0	1.5	0.20	0.6
1 000	0.0	0.0	0.0	1.0	0.20	0.6
2 000	-0.1	-0.1	-0.1	2.0	0.20	0.6
4 000	-0.4	-0.4	-0.1	3.0	0.20	0.6
8 000	-0.6	-0.6	-0.2	5.0	0.20	0.7

Date of Calibration : 24-27 Feb.2025

The results relate only to the items tested/calibrated or value assigned.
Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.5

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang, Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9009

Office/Laboratory
668 Mu 2 Tambon Bangpoomai, Amphoe Muang Samutprakan, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtc@tistr.or.th Website : www.tistr.or.th

Office
196 Phahonyothin Road, Ladyao, Chatuchak, Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827

NSC-TISI-TIS 17025
CALIBRATION 0037

THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-68/0160 **MTC No.** EEL. BP. 87/0168

5. Long-term stability

Time	Measured Value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Begin	94.0	0.0	0.3	0.10	0.1
End	94.0				

6. Frequency and time weightings at 1 kHz

6.1 Frequency weightings at 1 kHz

Frequency Weighting	Measured Value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
A-weight	94.0	0.0	0.2	0.20	0.2
C-weight	94.0	0.0	0.2	0.20	0.2
Flat	94.0	0.0	0.2	0.20	0.2

6.2 Time weightings at 1 kHz

Frequency Weighting	Measured Value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Fast	94.0	0.0	0.1	0.20	0.2
Slow	94.0	0.0	0.1	0.20	0.2
Leq	94.0	0.0	0.1	0.20	0.2

Date of Calibration : 24-27 Feb.2025

The results relate only to the items tested/calibrated or value assigned.
Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.5

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang, Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9009

Office/Laboratory
668 Mu 2 Tambon Bangpoomai, Amphoe Muang Samutprakan, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtc@tistr.or.th Website : www.tistr.or.th

Office
196 Phahonyothin Road, Ladyao, Chatuchak, Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827

NSC-TISI-TIS 17025
CALIBRATION 0037

THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-68/0160 **MTC No.** EEL. BP. 87/0168

7. Level linearity on the reference level range

Anticipated value (dB)	Measured Value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
122	122.0	0.0	1.1	0.30	0.3
121	121.0	0.0	1.1	0.30	0.3
120	120.0	0.0	1.1	0.30	0.3
119	119.0	0.0	1.1	0.30	0.3
114	114.0	0.0	1.1	0.30	0.3
109	109.0	0.0	1.1	0.30	0.3
104	104.0	0.0	1.1	0.30	0.3
99	99.0	0.0	1.1	0.30	0.3
94	94.0	0.0	1.1	0.30	0.3
89	89.0	0.0	1.1	0.30	0.3
84	84.1	0.1	1.1	0.30	0.3
79	79.1	0.1	1.1	0.30	0.3
74	74.1	0.1	1.1	0.30	0.3
69	69.1	0.1	1.1	0.30	0.3
64	64.0	0.0	1.1	0.30	0.3
59	59.0	0.0	1.1	0.30	0.3
54	54.0	0.0	1.1	0.30	0.3
49	49.0	0.0	1.1	0.30	0.3
44	44.0	0.0	1.1	0.30	0.3
39	39.0	0.0	1.1	0.30	0.3
34	34.1	0.1	1.1	0.30	0.3
33	33.1	0.1	1.1	0.30	0.3

Date of Calibration : 24-27 Feb.2025

The results relate only to the items tested/calibrated or value assigned.
Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.5

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang, Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9009

Office/Laboratory
668 Mu 2 Tambon Bangpoomai, Amphoe Muang Samutprakan, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtc@tistr.or.th Website : www.tistr.or.th

Office
196 Phahonyothin Road, Ladyao, Chatuchak, Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827

THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-68/0160 **MTC No.** EEL. BP. 87/0168

7. Level linearity on the reference level range

Anticipated value (dB)	Measured Value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
32	32.2	0.2	1.1	0.30	0.3
31	31.2	0.2	1.1	0.30	0.3
30	30.3	0.3	1.1	0.30	0.3

8. Level linearlity including the level range control

At reference sound level on the reference level range

Range	Anticipated value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
40-130	94.0	94.0	0.0	1.1	0.30	0.3
30-120	94.0	94.0	0.0	1.1	0.30	0.3
20-110	94.0	94.0	0.0	1.1	0.30	0.3
20-100	94.0	94.0	0.0	1.1	0.30	0.3

Date of Calibration : 24-27 Feb.2025

The results relate only to the items tested/calibrated or value assigned.
Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang, Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9009

Office/Laboratory
668 Mu 2 Tambon Bangpoomai, Amphoe Muang Samutprakan, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtc@tistr.or.th Website : www.tistr.or.th

Office
196 Phahonyothin Road, Ladyao, Chatuchak, Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827

NSC-TISI-TIS 17025
CALIBRATION 0037

THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-68/0160 **MTC No.** EEL. BP. 87/0168

8. Level linearlity including the level range control

At reference level at 5 dB greater than the under-range on a level range

Range	Anticipated value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
40-130	45.0	45.0	0.0	1.1	0.30	0.3
30-120	35.0	35.0	0.0	1.1	0.30	0.3
20-110	25.0	25.3	0.3	1.1	0.30	0.3
20-100	25.0	25.2	0.2	1.1	0.30	0.3
20-90	25.0	25.1	0.1	1.1	0.30	0.3
20-80	25.0	24.9	-0.1	1.1	0.30	0.3

9. Tone burst response

Time Weighting	Toneburst Duration, Tb (ms)	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Fast	200	115.8	-0.2	±1.0	0.20	0.3
	2	98.9	-0.1	+1.0; -2.5	0.20	0.3
	0.25	89.0	-1.0	+1.5; -5.0	0.20	0.3
Slow	200	109.3	-0.3	±1.0	0.20	0.3
	2	89.8	-0.2	+1.0; -5.0	0.20	0.3
SEL	200	109.9	-0.1	±1.0	0.20	0.3
	2	89.9	-0.1	+1.0; -2.5	0.20	0.3
	0.25	80.9	-0.1	+1.5; -5.0	0.20	0.3

Date of Calibration : 24-27 Feb.2025

The results relate only to the items tested/calibrated or value assigned.
Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang, Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9009

Office/Laboratory
668 Mu 2 Tambon Bangpoomai, Amphoe Muang Samutprakan, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtc@tistr.or.th Website : www.tistr.or.th

Office
196 Phahonyothin Road, Ladyao, Chatuchak, Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827

NSC-TISI-TIS 17025
CALIBRATION 0037

THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-68/0160 **MTC No.** EEL. BP. 87/0168

10. Peak C sound level

Number of cycles in test signal	Anticipated value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Complete cycle	125.4	125.5	0.1	3.0	0.20	0.35
Positive half cycle	124.4	124.3	-0.1	2.0	0.20	0.35
Negative half cycle	124.4	124.3	-0.1	2.0	0.20	0.35

11. Overload indication

Measured value (dB)		Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Positive one-half cycle	Negative one-half cycle				
132.5	132.5	0.0	1.5	0.20	0.25

12. High-level stability

Time	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Begin	129.0	0.0	0.3	0.10	0.1
End	129.0				

Calibrated by :

(Mr. Tawikiat Iamsamran)

Approved by :

(Mr. Prawate Kluaypa)
Director
Electrical and Electronic Standards Laboratory
Industrial Metrology and Testing Service Centre

Date of Calibration : 24-27 Feb.2025

Date of Issue : 28 Feb.2025

Ref : 2011268011400185005

End of Certificate

The results relate only to the items tested/calibrated or value assigned.
Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang, Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9009

Office/Laboratory
668 Mu 2 Tambon Bangpoomai, Amphoe Muang Samutprakan, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtc@tistr.or.th Website : www.tistr.or.th

Office
196 Phahonyothin Road, Ladyao, Chatuchak, Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827

ภาคผนวก จ-2

บริษัท ยูไนเต็ด แอนนาลิสต์ แอนด์ เอ็นจิเนียริ่ง คอนซัลแตนท์ จำกัด

List of Instruments Certification for Air & Noise Quality Analysis

No.	Instrument/Equipment	Parameter	Manufacturer	Model/Serial No.	Calibrator	Certification No.	Date of Calibration	Due date of Calibration	Remark
Stack									
1	Pre-Test Console	Total Suspended Particulate	Apex Instruments, USA.	XC-572-V 0707048	Envi Equipment Service Co., Ltd.	E25-070066	8 Jul 25	7 Jul 26	-
2	Flue gas Analyzer	Sulphur Dioxide Oxide of Nitrogen as Nitrogen Dioxide Carbon Monoxide Carbon Dioxide	Testo	Testo 350 60899698/701	Entech Industrial Sulution Co., Ltd.	G 680122	24 Feb 25	23 Feb 26	-

List of Instruments Certification for Water Quality Analysis

No.	Instrument/Equipment	Parameter	Manufacturer	Model/Serial No.	Calibrator	Certification No.	Date of Calibration	Due date of Calibration	Remark
Water									
1	pH Meter	pH	Horiba	LAQUA-PH210 HA4G0060	Technology Promotion Association (Thailand-Japan)	25CH1065	10 Sep 25	9 Sep 26	-

Envi Equipment Service Co., Ltd.
110/254 Moo 3, Tumbon Bang Rak Phatthana, Amphur Bang Bua Thong, Nonthaburi 11110
Tel. 098 362 9152, 089 478 7885
E-mail: sales@envi-ees.com

CERTIFICATE OF CALIBRATION

Customer	:	United Analyst and Engineering Consultant Co., Ltd.
Address	:	81 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Description of Equipment	:	Console meter
Manufacturer	:	Apex Instrument
Model Number	:	XC-572-V
Serial Number	:	0807048
ID./Control No.	:	UAE.ANV. 213/2551
Environment Conditions	:	Temperature (25 ± 2) °C
	:	Humidity (50 ± 15) % RH
Cal. Date	:	08/07/2025
Issue Date	:	08/07/2025

Calibration Method or Calibration Procedure Used

US EPA Method (United State Environmental Protection Agency)

This certificate is traceable to national standard, which realize the units of measurement according to the International System of Units (IS).

Result of Calibration

This certificate may not be reproduced other than in full except with prior Written approval of the Technical Manager, Envi Equipment Service Company Limited.

These reported uncertainties of measurement are expanded by a coverage factor of k=2, providing a 95% confidence level

Calibrated by : Mr. Sanya Sangnil

Approved by : (Mr. Mana Fuekhud)
Technical Manger

เอกสารไม่ควบคุม

METHOD 5 CONSOLE CALIBRATION
USING REFERENCE WET GAS METER W-NK-2.5-B-Z No.547425
5-POINT METRIC UNIT

Meter Console Information	
Console Model Number	XC-572-V
Console Serial Number	0807048
DGM Model Number	SK25EX
DGM Serial Number	00003811

Calibration Conditions			
Date	Time	08/07/2025	10:20 AM
Calibration Reference No.		SER25-070027	
Barometric Pressure		756.66	mmHg
Calibration Meter Gamma		1.001	

Factors/Conversions		
Std Temp	293	K
Std Press	760	mm Hg
K_1	0.386	
Console Leak Check		PASS

Calibration Data

Run Time	Metering Console					Calibration Meter			
Elapsed	DGM Orifice DH	Volume Initial	Volume Final	Outlet Temp Initial	Outlet Temp Final	Volume Initial	Volume Final	Outlet Temp Initial	Outlet Temp Final
(Q)	(P_m)	(V_{mi})	(V_{mf})	(t_{mi})	(t_{mf})	(Vwi)	(Vwf)	(t_{wi})	(t_{wf})
min	mm H_2O	m^3	m^3	°C	°C	m^3	m^3	°C	°C
11.50	13.0	1969.469	1969.609	31	31	322.96542	323.10612	29	29
11.60	13.0	1969.609	1969.749	31	31	323.10612	323.24610	28	28
8.10	26.0	1969.757	1969.897	30	30	323.25706	323.39652	27	27
8.07	26.0	1969.897	1970.037	30	30	323.39652	323.53548	27	27
13.60	40.0	1970.046	1970.326	30	30	323.54438	323.82228	26	26
13.63	40.0	1970.326	1970.606	30	30	323.82228	324.09872	26	26
9.90	70.0	1970.618	1970.898	30	30	324.10986	324.38576	26	26
9.87	70.0	1970.898	1971.178	31	31	324.38576	324.66104	25	25
8.82	90.0	1971.195	1971.475	31	31	324.67042	324.94510	25	25
8.83	90.0	1971.475	1971.755	31	31	324.94510	325.21908	25	25

เอกสารไม่ควบคุม

METHOD 5 CONSOLE CALIBRATION
USING REFERENCE WET GAS METER W-NK-2.5-B-Z No.547425
5-POINT METRIC UNIT

Meter Console Information	
Console Model Number	XC-572-V
Console Serial Number	0807048
DGM Model Number	SK25EX
DGM Serial Number	00003811

Calibration Conditions			
Date	Time	08/07/2025	10:20 AM
Calibration Reference No.		SER25-070027	
Barometric Pressure		756.66	mmHg
Calibration Meter Gamma		1.001	

Factors/Conversions		
Std Temp	293	K
Std Press	760	mm Hg
K_1	0.386	
Console Leak Check		PASS

Calibration Data

Results

Standardized Data				Dry Gas Meter				
				Calibration Factor		Flowrate		
Dry Gas Meter		Calibration Meter		Value	Variation	Std & Corr	.0212 m^3_{std}/min	Variation
($V_{m(std)}$)	($Q_{m(std)}$)	($V_{W(std)}$)	($Q_{W(std)}$)	(Y)	(△Y)	($Q_{m(std)(corr)}$)	(△$H_@$)	(△$H_@$)
m^3	m^3/min	m^3	m^3/min			m^3/min	mm H_2O	
0.135	0.012	0.136	0.012	1.005	0.018	0.012	40.562	-1.899
0.136	0.012	0.136	0.012	1.000	0.013	0.012	41.558	-0.903
0.136	0.017	0.136	0.017	0.995	0.008	0.017	40.797	-1.664
0.136	0.017	0.135	0.017	0.991	0.004	0.017	40.753	-1.708
0.274	0.020	0.271	0.020	0.990	0.003	0.020	44.532	2.071
0.274	0.020	0.270	0.020	0.984	-0.002	0.020	45.224	2.763
0.275	0.028	0.269	0.027	0.980	-0.007	0.027	42.140	-0.321
0.276	0.028	0.270	0.027	0.977	-0.009	0.027	41.905	-0.556
0.276	0.031	0.269	0.031	0.973	-0.013	0.031	43.376	0.915
0.276	0.031	0.268	0.030	0.971	-0.016	0.030	43.763	1.302
				0.987	Y Average		42.461	△H@ Average

Note: For Calibration Factor Y, the ratio of the reading of the calibration meter to the dry gas meter, acceptable tolerance of individual values from the average is ±0.02.
For △$H_@$, orifice pressure differential that equates to 0.75 cfm (0.0212 m^3/min) at standard temperature and pressure, acceptable tolerance of individual values from the average is ±0.2 inches (5.1mm) H_2O

เอกสารไม่ควบคุม

Meter Console Information	
Console Model Number	XC-572-V
Console Serial Number	0807048
DGM Model Number	SK25EX
DGM Serial Number	00003811

Calibration Conditions			
Date	Time	08/07/2025	10:20 AM
Calibration Reference No.		SER25-070027	
Barometric Pressure		756.66	mmHg
Calibration Meter Gamma		1.001	

Factors/Conversions		
Std Temp	293	K
Std Press	760	mm Hg
K_1	0.386	
Console Leak Check		PASS

Calibration Date: 8-7-2025 Calibration Reference No: SER25-070027

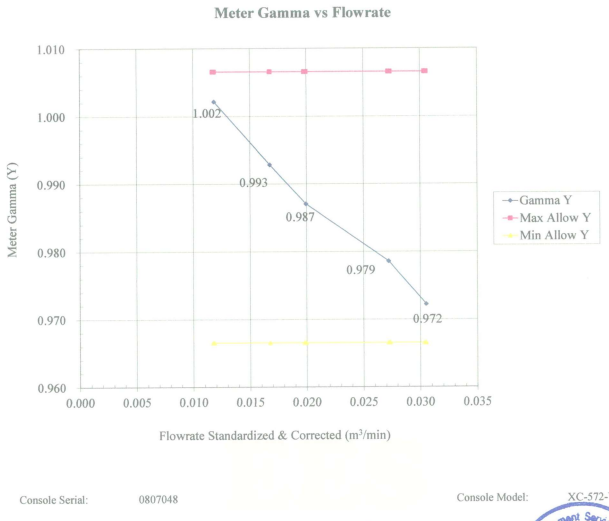

Console Serial: 0807048 Console Model: XC-572-V

เอกสารไม่ควบคุม

Meter Console Information	
Console Model Number	XC-572-V
Console Serial Number	0807048
DGM Model Number	SK25EX
DGM Serial Number	00003811

Calibration Conditions			
Date	Time	08/07/2025	10:20 AM
Calibration Reference No.		SER25-070027	
Barometric Pressure		756.66	mmHg
Calibration Meter Gamma		1.001	

Factors/Conversions		
Std Temp	293	K
Std Press	760	mm Hg
K_1	0.386	
Console Leak Check		PASS

Calibration Date: 8-7-2025 Calibration Reference No: SER25-070027

Meter Pressure vs Flowrate

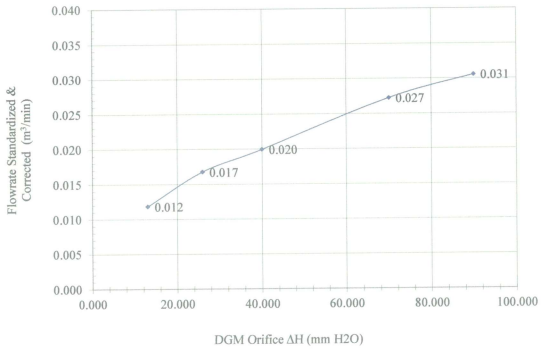

Console Serial: 0807048 Console Model: XC-572-V

EES Engineering Equipment Service Co., Ltd.
เอกสารไม่ควบคุม

THERMOCOUPLES SYSTEM CALIBRATION

Sampling System Equipment Information	
Console Model Number	XC-572-V
Console Serial Number	0807048
DGM Model Number	SK25EX
DGM Serial Number	00003811
Meter Box Model Number	JENCO 765 KF
Meter Box Serial Number	JC 08944

Calibration Conditions			
Date	Time	08/07/2025	00:30 PM
Calibration Reference No.		SER25-070027	
Reference Thermometer		DIGICON	
Serial Number		183169105	

Results										
Console Thermocouple Simulator										
Channel and test point	Meter Box Channel Temperature Reading (°C)									
	-18.0	25.0	38.0	93.0	149.0	260.0	371.0	482.0	593.0	1038.0
Stack	-19.0	24.0	37.0	92.0	148.0	258.0	370.0	481.0	593.0	1038.0
Aux	-19.0	24.0	37.0	92.0	148.0					
Probe	-19.0	24.0	37.0	92.0	148.0					
Filter	-19.0	24.0	37.0	92.0	148.0					
Oven	-19.0	24.0	37.0	92.0	148.0					
Exit	-19.0	24.0	37.0							

Tolerance Range

Stack	± 1.50%	Absolute	Meter	± 3.0 °C
Probe	± 3.0 °C		Exit	± 2.0 °C
Filter	± 3.0 °C			

EES Engineering Equipment Service Co., Ltd.
เอกสารไม่ควบคุม

ENTECH Where Solutions Begin

Calibration Certificate

NSC-TIS-TIS 17025 CALIBRATION 0157

Certificate No: G 680122
Date of issue : 25-Feb-25

Instrument description : Flue Gas Analyzer
Instrument model : Testo 350 NEW
Instrument serial no. : 60899698/701
Control unit serial no. : 03099393/701
ID no. or control no. : UAE.EFM.008/2560
Manufacturer : Testo SE & Co. KGaA
Probe description : -
Probe model : -
Probe serial no. : -
Customer name : UNITED ANALYST CONSULTANT CO.,LTD.
Customer address : 81 SOI UDOMSUK41,SUKHUMVIT ROAD,BANGCHAK PRAKANONG BANGKOK 10260

Total pages of certificate : 2 Pages
Receiving no. : L-250557
Receiving date. : 18-Feb-25
Parameter of calibration : Gas Calibration(Oxygen 2.50,9.984,21.02 %vol, Carbon Monoxide 80.45,302,1007 ppm) Nitrogen Dioxide 30.68,81.8,202.6 ppm, Nitric Oxide 30.0,151.8,322.5 ppm, Sulphur Dioxide 50.36,100.7,600.8 ppm)
Condition of UUC. : Used
Ambient condition : All of the Measurment ware caried out the stabilized labotary
Temperature : 23 ±5 °C
Humidity : 55 ± 15 %RH
Calibration place : 17/121 Soi Ngamwongwan 47 Yaek 48, Toongsonghong, Laksi, Bangkok 10210
Calibration procedure no : This instrument was calibrated by comparison with Standard gas mixture according to calibration Work Instruction no. WI-CL-28-C

The calibration certificate expanded uncertainty of measurement is stated as the standard uncertainty of measurement Multiplied by coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.
This certificate is applied only to item under test Environmental condition.
This Calibration Certificate may not be reporduced other than in full except with the permission of the issuing laboratory. Calibration certificates without signature and seal not valid and The results relate only to the items tested/calibrated.
This calibration certificate documents are traceability to national standards, which realize measurement according to the International System of Units (SI).

Date of calibration : 24-Feb-25

Mr. Kwanchai Khamdoung
Calibration Technician

Mrs. Nongluck Wongsettee
Technical Manager

เอกสารไม่ควบคุม

Entech Industrial Solution Co.,Ltd.
17/121 Soi Ngamwongwan 47 Yaek 48, Toongsonghong, Laksi, Bangkok 10210 THAILAND Tel. 0-2779-8888 Calibration@entech.co.th
Tax ID : 0105536035591 www.entech.co.th

ENTECH Where Solutions Begin

Calibration Certificate

NSC-TIS-TIS 17025 CALIBRATION 0157

Certificate No.: G 680122

Standard References (Table 1)

Standard	Certificate No.	Vendor	Due date
Oxygen (O2) 2.50 % Vol	2412/23	Lindc	27 Aug 27
Oxygen (O2) 9.984 % Vol	CG-0113-24	Nimt	01-Aug-29
Oxygen (O2) 21.02 % Vol	CG-0041-22	Nimt	10-Feb-27
Carbon monoxide (CO) 80.45 ppm	CG-0132-24	Nimt	10-Sep-29
Carbon monoxide (CO) 302 ppm	1915/23	Linde	16-Jun-25
Carbon monoxide (CO) 1007 ppm	1870/24	Linde	17-Jun-26
Nitrogen Dioxide (NO2) 30.68 ppm	2832/24	Linde	08-Sep-26
Nitrogen Dioxide (NO2) 81.8 ppm	2330/24	Linde	01-Aug-26
Nitrogen Dioxide (NO2) 202.6 ppm	3794/24	Linde	23-Dec-26
Nitric Oxide (NO) 30.0 ppm	CG-0065-24	Nimt	06-May-26
Nitric Oxide (NO) 151.8 ppm	0404/25	Linde	09-Feb-27
Nitric Oxide (NO) 322.5 ppm	1974/23	Linde	17-Jul-25
Sulphur Dioxide (SO2) 50.36 ppm	2004/23	Linde	17-Jul-25
Sulphur Dioxide (SO2) 100.7 ppm	2662/24	Linde	25-Aug-26
Sulphur Dioxide (SO2) 600.8 ppm	2003/23	Linde	17-Jul-25

Measured room conditions
Temperature : 23.5 °C Humidity : 62.9 %RH Pressure : 1013.1 mbar
Calibration conditions
Gas Temperature : 23 °C Flow rate : 1,300 ml/min Gas pressure : 1016.9 mbar

Calibration Results (Without adjustment) (Table 2)

Parameter of Standard	Standard Values	Mean of UUC	Error	Uncertainty (±)
O2 (%Vol)	2.50	2.44	-0.06	0.15
O2 (%Vol)	9.984	9.91	-0.074	0.20
O2 (%Vol)	21.02	21.11	0.09	0.30
CO (ppm)	80.45	80	-0.45	3.0
CO (ppm)	302	303	1	6.0
CO (ppm)	1007	1009	2	12
NO2 (ppm)	30.68	32.3	1.62	8.0
NO2 (ppm)	81.8	82.5	0.7	8.0
NO2 (ppm)	202.6	203.4	0.8	12
NO (ppm)	30.0	30	0.0	8.0
NO (ppm)	151.8	153	1.2	8.0
NO (ppm)	322.5	324	1.5	12
SO2 (ppm)	50.36	50	-0.36	6.0
SO2 (ppm)	100.7	101	0.3	6.0
SO2 (ppm)	600.8	603	2.2	13

Remark : 1 cmol/mol = 1 %vol. 1 µmol/mol = 1 ppm., Sensor CO, NO2, SO2 New.

End of Report

เอกสารไม่ควบคุม

Entech Industrial Solution Co.,Ltd.
17/121 Soi Ngamwongwan 47 Yaek 48, Toongsonghong, Laksi, Bangkok 10210 THAILAND Tel. 0-2779-8888 Calibration@entech.co.th
Tax ID : 0105536035591 www.entech.co.th

TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL.0-2717-3000-29 FAX.0-2719-9484

ilac-MRA

NSC-TISI-TIS17025
CALIBRATION 0008

Certificate of Calibration

Cert.No.: 25CH1065
Page.: 1 of 3

Equipment : pH Meter
Manufacturer : Horiba
Model : LAQUA-PH210
Serial No. : HA4G0060
ID No. : UAE.EFM.202/2564(EFM.pH.10/64)
Condition As-Received: Used Item
Received Date : 09 September 2025
Calibration Date : 10 September 2025
Reference : 2509-0327WSC-1
Submitted by : United Analyst and Engineering Consultant Co.,Ltd.
3 Soi Udomsuk 41, Sukhumvit Road, Bangchak,
Phrakhanong, Bangkok 10260
Ambient Temperature : (25 ± 2.5) °C
Relative Humidity : (50 ± 15) %
Calibration Procedure : In - house method :
- CP-CH5 by direct measurement with DC voltage standard and direct measurement with certified reference material (CRM)
- CP-CH8 by comparison with temperature standard

Calibrated by : Walalak Sirithean

Approved by : Saithip
Approved Signatory

( ) Chakrit Waewwanjua
( ) Ponpan Paipim
(✓) Saithip Meangmai

Issue Date : 12 September 2025

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

เอกสารไม่ควบคุม

Condition of this calibration result

1. Reference Standard Instrument

Instrument	Serial No.	ID No.	Cert. No.	Due Date
1) Document Process Calibrator	54030049	130RC116	25E2743	25 Aug 2026
2) Ref. Standard Thermometer	4982054	110RC044	25I708	03 July 2026

- This measurement result is traceable to SI throught Technology Promotion Association (Thailand - Japan)

2. Certified Reference Materials :The measurement results are traceable to SI through Hach Lenge GmbH Ltd., Deutsche Akkreditierungsstelle, Accredited No.D-RM-15184-01-00
:The measurement results are traceable to SI through CPA chem Ltd., ANSI-ASQ National Accreditation Board, Accredited No. AR-1835

Buffer Solution	Manufacturer	Lot No.	Exp. date
pH 4.007	CPA chem	1114384	12 June 2027
pH 6.999	Hach Lenge GmbH	C03273	13 May 2027
pH 10.010	CPA chem	1114385	08 June 2026

3. This certificate is valid only to the item calibrated on date and place of calibration.

Calibration Results

Function : mV Measurement

Performing standard curve by Document Process Calibrator at pH (4,7)(7,10)

Unit Under Calibration	Nominal Value	Standard Voltage Input	Actual Reading		Uncertainty of Measurement	Coverage factor
	pH	mV	mV	pH	(±mV)	k
pH Meter	4.00	177.48	177.1	4.01	0.058	2.00
S/N.: HA4G0060	7.00	0.00	0.0	7.00	0.058	2.00
	7.00	0.00	0.0	7.00	0.058	2.00
	10.00	-177.48	-177.0	10.01	0.058	2.00

เอกสารไม่ควบคุม

Calibration Results

Function : pH Measurement

Performing three buffers standard curve by using buffer nominal pH (4,7)(7,10)

Unit Under Calibration	Standard pH Buffer Solution	Actual pH Reading	Actual mV Reading (mV)	Uncertainty of pH Measurement (±)	Coverage factor k
pH Electrode	4.007	4.01	173.0	0.0079	2.00
S/N.: Q9BF0097	6.999	7.00	-2.2	0.0085	2.00
	6.999	7.01	-2.1	0.0085	2.00
	10.010	10.01	-173.7	0.0096	2.00

Function : Temperature Measurement

(*) Without adjustment

This equipment was connected with Temperature Probe;
- Model : 9652-10D
- Serial No. : Q9BF0097

Dimension of probe
- Length : 107 mm.
- Diameter : 15 mm.
- Immersion Depth : 85 mm.

Calibration Point (°C)	Standard Temperature (°C)	UUC* Reading (°C)	Error (°C)	Uncertainty of measurement (± °C)	Coverage factor k
15.0	14.998	15.0	0.002	0.13	2.00
30.0	30.002	30.0	-0.002	0.13	2.00
45.0	45.002	44.9	-0.102	0.13	2.00

Remark - UUC* = Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

เอกสารไม่ควบคุม

List of Instrument Certificates for Environmental Quality Analysis

No.	Instrument/Equipment	Parameter	Manufacturer	Model/Serial No.	Calibrator	Certification No.	Date of Calibration	Due date of Calibration*
1	Atomic Absorption Spectrometer	CHROMIUM TRIVALENT IRON	Agilent Technologies	AA240FS / MY13160001	Agilent Technologies (Thailand) Co.,Ltd.	Preventive Maintenance Checklist	30/1/2025	29/1/2026
2	SCT Meter	CONDUCTIVITY (umhos/cm)	Horiba	LAQUA-EC210 / HC9L0013	Technology Promotion Association (Thailand-Japan)	25CH167	5/2/2025	3/2/2026
3	Ion Selective Electrode Meter	FLUORIDE	Thermo Fisher Scientific, Indonesia And USA	Orion Star A214 / X36836	Science Tech Co.,Ltd.	ST014/25	20/5/2025	19/5/2026
4	Kjeltec System Distilling Unit	TOTAL KJELDAHL NITROGEN	Foss Tecator (Labtec)	KT200 / 91790524	FOSS South East Asia	13319	27/1/2025	26/1/2026
5	Kjeltec Distillation Unit	TOTAL KJELDAHL NITROGEN	FOSS	Kjeltec 8100 / 91889052	FOSS South East Asia	13854	24/2/2025	23/2/2026
6	Spectrophotometer	COLOUR (pH 7.0) COLOUR (pH Sample)	Agilent	Cary 60 G6860A / MY15410009	DQE Services Co.,Ltd.	SP25-019	26/5/2025	25/5/2026
7	UV-VIS Spectrophotometer	NITRATE PHOSPHATE	Hitachi	U-2900 / 21E22-009	DQE Services Co.,Ltd.	SP25-021	26/5/2025	25/5/2026

Due Date of Calibration* : Based on the annual calibration plan. At least 1 time per year.

Agilent CrossLab
From Insight to Outcome

Agilent 55 240 280 Series Atomic Absorption Spectroscopy Systems

Preventive Maintenance Checklist

Agilent Preventive Maintenance provides factory recommended service for your analytical systems to assure reliable operation and the accuracy of your results.

Delivered by highly trained and certified service engineers using genuine Agilent parts and supplies, Agilent Preventive Maintenance provides everything you need to reduce unplanned downtime and keep your systems operating at their peak. This checklist will be completed at the end of the service and provided to you as a record of the installation.

Note: While non-current production AA instrument and or accessory models are not covered specifically in this document it can be used as a basic reference.

For more information about Agilent Technologies services please visit our web site using the following URL http://www.agilent.com/en-us/services

Introduction

Customer Information

1 Customers should provide all necessary operating supplies upon request of the engineer.

2 A customer representative should be available to the engineer while performing the preventive maintenance procedures.

3 Any parts, not included in the Parts Lists section of this document, are not part of the recommended Preventive Maintenance service, nor are they included in the price of this service.

4 If a system requires the use of extra or special procedures and/or parts for the maintenance service, then these must be ordered separately and charged as a repair, which may incur additional costs.

Revision: 10.00, Issued: November 2021

© Agilent Technologies, Inc. 2021

Agilent
เอกสารไม่ควบคุม

Important Customer Web Links

- For more information about *Agilent Technologies services*, please visit our website using the following URL: http://www.agilent.com/en-us/products/crosslab-instrument-services/service-repair
- To access *Agilent University*, visit http://www.agilent.com/crosslab/university/ to learn about training options, which include online, classroom and onsite delivery.
  A training specialist can work directly with you to help determine your best options.
- A useful *Agilent Resource Center* web page is available, which includes short videos on maintenance, quick lists of consumables for new instruments, and other valuable information. Check out the Resource Page here: https://www.agilent.com/en-us/agilentresources
- Need technical support, FAQs, supplies? – visit our *Support Home page* at http://www.agilent.com/search/support
- Get answers. Share insights. Build connections:
  Join the *Agilent Community* at https://community.agilent.com/welcome

Service Engineer's Responsibilities

- Contact the customer and ensure that all necessary supplies are available before the preventive maintenance visit.
- Confirm the ability of the instrument to deliver continued safe operation as established via the Agilent AA safe operation flow chart. (Refer directly to the AA 55/240/280 Preventive Maintenance Scope of Work to make this decision.)
- Only select those pages that relate to the system or module being serviced.
- Complete empty fields with the relevant information.
- Complete the relevant checkboxes in the checklist using either a "X" or tick mark "✓".
- Check "Section not applicable" check boxes to indicate services/tasks not delivered, as appropriate.
- Complete the Preventive Maintenance service in the order of the tasks listed.
- Complete the Service Review section together with the customer.
- Complete the fields for page numbers at the foot of each selected page
- Complete the total number of pages field in the Service Completion section
- Ask the customer to sign the Service Completion section including the customer's and your signature.

This information is subject to change without notice.

Revision: 10.00, Issued: November 2021

© Agilent Technologies, Inc. 2021

Agilent
เอกสารไม่ควบคุม

Instrument Maintenance

System Information

❑ Check this box if an instrument configuration report is attached instead of completing the table.

Instrument System Name and ID	240 FS AAS
Instrument System Site and Location	United Analyst and Engineering Consultant

List System Component Product Numbers	List the Serial Numbers of each Component
1. G 8432 A	MY 13160001
2.	
3.	
4.	
5.	
6.	
7.	
8.	
9.	

Preparation, Safe operation and Initial performance checks

Revision: 10.00, Issued: November 2021

© Agilent Technologies, Inc. 2021

Agilent
เอกสารไม่ควบคุม

❑ Agilent AA safe operation flow chart inspections (to determine if the PM can be performed).

NOTE: If by following the flow chart the instrument is deemed to be unsafe for continued use you MUST NOT continue PM work. Inform the customer immediately of the Agilent recommendation that use of the instrument be discontinued.

☑ Discuss any specific issues with the customer before starting.

❑ For HF application systems, if standard sample introduction system was not installed, ask the customer to install it. N/A

☑ Review the instrument logbook for recorded problems and comments.

☑ Save instrument control settings before starting the procedure.

☑ Perform a general inspection of the system for cleanliness.

☑ Check for proper installation of parts, assemblies, sensors etc.

☑ Check system for required installation of components, settings as defined by current Service Notes

☑ Check for required firmware updates and verify with customers if they would like them installed.

☑ Use SVD to perform a Full Wavelength Scan for Cu HCL - "As found test_1"

☑ Perform a Basic Cu ABS test - "As found test_2"

☑ Print the Details page or screen captures of the test results and attach to the end of this checklist.

Revision: 10.00, Issued: November 2021

© Agilent Technologies, Inc. 2021

Agilent
เอกสารไม่ควบคุม

Preventive Maintenance Procedures

FLAME SYSTEM section

☐ *Section not applicable*

Electronic components

- ☑ Review and confirm instrument configuration data in SVD
- ☑ Confirm power supply voltages using the *SVD Power Supply diagnostic*.
- ☑ For Dual Beam instruments - Confirm RBC frequency using the *SVD RBC frequency diagnostic*.

Mechanical components

- ☑ Check the burner adjuster controls for complete and free movement. If the burner adjuster needs lubrication, use Molykote 321 or mineral-based molybdenum disulphide grease.
- ☑ Run SVD tests to exercise all motor drives over the full range of their travel:
  - ☑ Monochromator drive
  - ☑ Slit drive
  - ☑ Lamp selector
  - ☐ ABA

Optics components

- ☑ Check that external optical surfaces are clean – Clean or replace as required.
- ☑ Use SVD and perform *Mono Wavelength Correction.*
- ☑ Use SVD and perform *Slit Calibration.*
- ☑ Use SVD and perform *Grating Squareness Diagnostic.*
- ☑ Use SVD and perform *Zero Order Offset/Mono Correction.*
- ☑ Use SVD and perform *Wavelength Repeatability.*
- ☑ Physically inspect selected HC lamps (customer to supply per their choice) and measure the % Gain for each lamp. Advise customer if lamps are showing emission degradation due to age.
- ☑ Check that the signal energy of the D2 and HC lamps track properly. Advise customer if their D2 lamp is showing emission degradation due to age.

© Agilent Technologies, Inc. 2021

Agilent
เอกสารไม่ควบคุม

Agilent CrossLab From Insight to Outcome
Instrument Preventive Maintenance Checklist

Sample Introduction and Atomization

- ☑ Inspect the burner interlock plate to ensure that the interlock pin is secure and correct for the burner type.
- ☑ Clean the burner slot with a clean white card.
- ☑ Check the uniformity of the slot width.
- ☑ Clean the burner if required.
- ☑ Change the burner o-ring.
- ☑ Clean the nebulizer, spray chamber and liquid trap.
- ☑ Change all o-rings and seals in the nebulizer, nebulizer block and spray chamber.
- ☑ Check that the pressure relief bung releases readily.
- ☑ Change o-rings on the fuel and oxidant delivery barbs
- ☑ Leave the liquid trap EMPTY and verify the flame will not ignite in this state.
- ☑ Refill liquid trap and check that overfill drains freely into the drain/waste tube.
- ☑ Check the drain/waste tube for good drainage. It should not have tight bends, kinks or loops and the lower end must be above the liquid level in the waste vessel
- ☑ Check and clean the igniter electrode

Gas handling components and safety interlocks

- ☑ Pressure test for leaks
- ☑ Leak test gasbox internal components and connections
- ☑ Check safety interlock status and operation using the *SVD interlock monitoring diagnostic.*

Analytical performance for Flame systems

- ☑ Ignite a flame.
- ☑ Check that you can adjust the nebulizer uptake rate from 4 to 6.5 mL per minute.
- ☑ Optimize the instrument ready to perform Cu sensitivity test.
- ☑ Create a manual method to perform a Basic Cu ABS test - "Final Performance Testing "
- ☑ Run a PM completed sensitivity test for a 5 ppm copper sample and record the results in the AA PM Performance test results and measurements table.

Revision: 10.00, Issued: November 2021

© Agilent Technologies, Inc. 2021

Agilent
เอกสารไม่ควบคุม

Agilent CrossLab From Insight to Outcome
Instrument Preventive Maintenance Checklist

FURNACE SYSTEM section

☑ *Section not applicable*

Electronic components

- ☐ Review and confirm instrument configuration data in SVD
- ☐ Confirm power supply voltages using the *SVD Power Supply diagnostic*.

Mechanical components

- ☐ Run SVD tests to exercise all motor drives over the full range of their travel:
  - ☐ Monochromator drive
  - ☐ Slit drive
  - ☐ Lamp selector

Optics components

- ☐ Check that external optical surfaces are clean – Clean or replace as required.
- ☐ Use SVD and perform *Mono Wavelength Correction.*
- ☐ Use SVD and perform *Slit Calibration.*
- ☐ Use SVD and perform *Grating Squareness Diagnostic.*
- ☐ Use SVD and perform *Zero Order Offset/Mono Correction.*
- ☐ Use SVD and perform *Wavelength Repeatability.*
- ☐ Physically inspect selected HC lamps (customer to supply per their choice) and measure the % Gain for each lamp. Advise customer if lamps are showing emission degradation due to age.

Gas handling, water system and workhead component checks

- ☐ Inspect the GTA workhead gas hoses and connections for leaks.
- ☐ Pressure test for gas leaks
- ☐ If the cooler system is accessible (stand-alone) check for correct operation and coolant/water level – this includes any temperature and pressure settings plus filter cleaning (air flow and water).
- ☐ Inspect the GTA workhead water hoses and connections for leaks.
- ☐ Check all graphite components and replace if necessary.

Revision: 10.00, Issued: November 2021

© Agilent Technologies, Inc. 2021

Agilent
เอกสารไม่ควบคุม

Agilent CrossLab From Insight to Outcome
Instrument Preventive Maintenance Checklist

  - ☐ Tube
  - ☐ Electrodes
  - ☐ Shroud
- ☐ Check and clean the end windows on the workhead.
- ☐ Check safety interlock operation.

Analytical performance for Furnace systems

- ☐ Optimize the instrument ready to perform Cu sensitivity test.
- ☐ Run the sensitivity test for a 25 ppb copper sample and record the results in the results table.

PSD autosampler accessory for Furnace systems

☑ *Section NOT Applicable*

- ☐ Check condition of the PSD capillary – replace if necessary
- ☐ Check condition and operation of PSD syringe – ensure it does not have air locks and bubbles.
- ☐ Change PSD rinse bottle o-ring.
- ☐ Check and clean the rinse vessel.
- ☐ Check the drain tube for good drainage. It should not have tight bends, kinks or loops and the lower end must be above the liquid level in the waste vessel.
- ☐ Ensure that the waste vessel is suitable for use with the furnace system.

Sample introduction pump system (SIPS) accessory

☑ *Section NOT Applicable*

- ☐ Re-torque screws securing the hubs, presser arms and pump rotors.
- ☐ Adjust each roller so that it rotates freely.
- ☐ Wipe clean the pump rotor rollers and pump bands with a dry clean cloth.
- ☐ Ensure that the presser arms and the surfaces near the pump are free from dirt and spills.
- ☐ Remove the pump module rear cover and check for the incursion of liquids and any signs of corrosion.
- ☐ Re-torque the nuts that fasten the motor mounting plates to the chassis.
- ☐ Check clips securing the diluents holder and replace if necessary.
- ☐ Disconnect, clean T-piece, and reassemble the tubing using the following steps.

Revision: 10.00, Issued: November 2021

© Agilent Technologies, Inc. 2021

Agilent
เอกสารไม่ควบคุม

- ❑ Remove the T-piece by disconnecting the pump tubes, the pump bands and all other tubing.
- ❑ Place the T-piece in an ultrasonic bath containing strong detergent 1-5% Decon 30 or similar, for approximately 5-10 minutes.
- ❑ Wash the T-piece under a tap with a strong flow of water.
- ❑ Rinse with distilled water through all of the inlets in the reverse direction to normal sample flow.
- ❑ Reassemble.

Sample preparation system (SPS 4) accessory

☑ *Section NOT Applicable*

The Agilent SPS 4 autosampler is designed to need minimal maintenance.

The following maintenance requirements are suggested to maintain the performance of the autosampler.

- ❑ Cleaning the spill tray, rack location mat, end frames and chassis accessories with a damp soft cloth and diluted mild detergent.
- ❑ Cleaning the autosampler cover panels with domestic window cleaner.
- ❑ Checking the X- axis and Z- axis drive belts for cracks, splits, damaged teeth, excessive fraying, color changes or degradation from fumes..
- ❑ Check the X- axis, Theta- axis and Z- axis FFC cables for cracks, incorrect positioning, damaged edge or damaged connectors.

NOTE: The autosampler requires no extra lubrication throughout its lifetime.
For further details refer to the SPS 4 service manual G8410-90050.

Sample preparation system (SPS 3) accessory

☑ *Section NOT Applicable*

- ❑ Check the x-axis and z-axis timing belts – Replace if there is are any cracks, splits or color deterioration and belt tension.
- ❑ Check belt tensions - adjust if required
- ❑ Check the lubrication pad for single x-axis shaft. If pad is dry or customer has observed any vibration or erratic movements of the x-axis carriage, add 1 mL of Dow Corning 200 ® Fluid, 200 CS into the well.
- ❑ Check the auto-sampler ability to find tube positions - Calibrate if required.
- ❑ Clean the exterior surfaces of the accessory with soft lint free cloth. This cloth can be dampened with warm water or a mild detergent. Do not use organic solvents or abrasive cleaning agents.

© Agilent Technologies, Inc. 2021

Agilent
เอกสารไม่ควบคุม

Agilent CrossLab From Insight to Outcome
Instrument Preventive Maintenance Checklist

Vapor generation accessory VGA (hydride generator)

❑ *Section NOT Applicable*

- ❑ Inspect VGA gas supply hose.
- ❑ Inspect/replace VGA pump tubing.
- ❑ Check low gas pressure interlock setting– adjust if required.
- ❑ Check precision orifice gas flow setting – adjust if required.
- ❑ Check gas regulator pressure to 46 psi (325 kPa) – adjust if required.
- ❑ Clean the exterior surfaces of the accessory with soft lint free cloth. This cloth can be dampened with warm water or a mild detergent. Do not use organic solvents or abrasive cleaning agents.

UltrAA lamp accessory (external)

☑ *Section NOT Applicable*

- ❑ Check the condition of the power cable.
- ❑ Clean the exterior surfaces of the accessory with soft lint free cloth. This cloth can be dampened with warm water or a mild detergent. Do not use organic solvents or abrasive cleaning agents.

Restore System

- ❑ If you have altered the customer's instrumentation during the course of PM, restore to the original status to allow the customer to conduct their normal activities (e.g., reload the customer's method.)

Guidance

If the PM service is performed prior to a qualification service, then use the qualification procedure as a guide for final instrument set up and checkout.

Revision: 10.00, Issued: November 2021

© Agilent Technologies, Inc. 2021

Agilent
เอกสารไม่ควบคุม

Agilent CrossLab From Insight to Outcome
Instrument Preventive Maintenance Checklist

Signature Page

Service Review

- ☑ Attach available reports/printouts of all tests to this documentation.
- ☑ Record the Preventive Maintenance service activity in the customer's records/logbook.
- ☑ Update/reset instrument maintenance counters as appropriate.
- ☑ Affix the PM sticker to the system or instrument logbook based on the customer's request.
- ☑ Complete the Service Engineer Comments section if there are additional comments.
- ☑ Review this service, parts replaced, and test results obtained with the customer.
- ☑ If the instrument firmware was updated, record the details of the change in the Service Engineer's Comments box or if necessary, in the customer's IQ records.

Test Results

Test Description	Expected Test Result	Actual Test Result
Flame optics PMT Gain test		
For copper at 324.8 nm, 4 mA, 0.5 nm slit width	< 55 %	49%
Flame performance test with 5 ppm copper sample		
Air /acetylene, mixing paddle removed	Abs value > 0.5	0.5598
Air /acetylene, mixing paddle installed. 10 replicates	%RSD < 1.0	0.2%
Deuterium furnace optics PMT Gain test		
For copper at 324.8 nm, 4 mA, 0.5 nm slit width	< 55 %	–
Deuterium furnace performance test with 25 ppb copper sample (324.8 nm)		
Precision %RSD	≤ 4.0%	–
Abs value	≥ 0.15	–
Zeeman furnace analytical performance: 25 ppb copper sample (327.4 nm)		
Precision %RSD	≤ 4.0%	–
Abs value	≥ 0.10	–
MSR%	≥70 %	–

Revision: 10.00, Issued: November 2021

© Agilent Technologies, Inc. 2021

Agilent
เอกสารไม่ควบคุม

Agilent CrossLab From Insight to Outcome
Instrument Preventive Maintenance Checklist

AA consumable and parts list table

Part Description	Part Number	Product/Model # where used	PM supplied or Consumable	Instrument-Type
Test Solution – Cu 5ppm solution	6610030100	50 55 140 240 280	PM supplied	Common
Test Solution - Blank solution	5190-7001	50 55 140 240 280	PM supplied	Common
Copper, 1000 ug/ml, 100ml	5190-8279	50 55 140 240 280	*	Common
Kit, Mk 7 O-rings, aqueous, complete set	9910093400	50 55 140 240 280	PM supplied	Flame
Organic Kit	9910093500	50 55 140 240 280	PM supplied	Flame
Wire Nebulizer Cleaning	9910024700	50 55 140 240 280	consumable	Flame
Tubing-Capillary Std Nebs	9910024800	50 55 140 240 280	consumable	Flame
Capillary Tube Hivac Neb (3) (organics only)	9910044000	50 55 140 240 280	consumable	Flame
Glass impact beads (5/pk)	9910025700	50 55 140 240 280	consumable	Flame
Teflon impact beads (5/pk): (organics only)	9910053300	50 55 140 240 280	consumable	Flame
Burner cleaning strip (100/pk)	9910053900	50 55 140 240 280	consumable	Flame
Window UV silica – round (right side)	2010082600	50 55 140 240 280	PM supplied	Common
Window UV silica – rectangular (left side)	2010082500	50 55 140 240 280	PM supplied	Common
Pad adhesive window (round)	4910012700	50 55 140 240 280	PM supplied	Common
Pad adhesive window (rectangular)	4910012800	50 55 140 240 280	PM supplied	Common
Electrode kit (1 pr) (D2)	6310003400	GTA120	PM supplied	Furnace
Shroud (D2)	6310003100	GTA120	PM supplied	Furnace
Zeeman electrode kit (1 pr)	6310003500	GTA120	PM supplied	Furnace
Zeeman shroud	6310003600	GTA120	PM supplied	Furnace
O-ring PSD rinse bottle	6910025900	PSD120	PM supplied	Furnace

* For engineers who only service AA instruments 5190-8279 can be used as a cheaper alternative for 6610030100.

Items classified as PM supplied in the above table are included in the standard PM

Those classified as consumable should be provided by the customer or charged to the customer if supplied by the Agilent service engineer.

Revision: 10.00, Issued: November 2021

© Agilent Technologies, Inc. 2021

Agilent
เอกสารไม่ควบคุม

Agilent CrossLab
From Insight to Outcome

Instrument Preventive Maintenance Checklist

Service Engineer Comments (optional)

If there are any specific points you wish to note as part of performing the installation or other items of interest for the customer, please write in this box.

Service Completion

Service request number 6007549143

Date service completed 30 Jan 2025

Agilent signature Kanyakorn S.

Customer signature Wanida Y.

Total number of pages in this document 13

Revision: 10.00, Issued: November 2021

© Agilent Technologies, Inc. 2021

Agilent

เอกสารไม่ควบคุม

SVD Results Report

VARIAN

Report ID:2 Diagnostic Start Time:1/30/2025 9:14:26 AM Diagnostic End Time:1/30/2025 9:46:06 AM

Customer: UAE **Service Engineer:** Kanyakorn S.

Address: Soi Udomsuk 41, Sukhumvit Rd. Bangkok **Contact Details:** 026376363#1

Instrument Configuration

Configuration:

Serial Number:	MY13160001	**Turret Type:**	Automatic
Instrument Model:	Varian AA140/240/280	**Number Of Lamps:**	4
Flame Instrument:	True	**Mono Type:**	Automatic
Furnace Instrument:	True	**Gasbox Type:**	'Y' Gas Box
Zeeman Present:	False	**Auto Burner Adjuster:**	False
Internal Zeeman:	False	**Mains Frequency:**	50
Internal UltrAA:	False	**Firmware Version:**	2.11
Optics Type:	Double Beam	**Photomultiplier Type:**	Normal(900nm)
D2 BG Correction Fitted:	True	**PWB Version:**	45
Boot Block Version:	1.09		

EEPROM Data:

Instrument Run Hours:	69818.180	**D2 Run Hours:**	53396.500
Zero Wavelength Offset:	30.133	**D2 Serial Number:**	not set !
Mono Correction:	0.770	**D2 Install Date:**	1/1/1970
Flame Hours:	32441.834	**D2 Original Intensity:**	1.000
		D2 Last Intensity:	475.000

เอกสารไม่ควบคุม

Frequency:

Averaging Period: 30.0

Datapoint Count: 20

Upper Limit: 51.00

Average Frequency: 50.00

Highest Measured Frequency: 50.00

Lower Limit: 49.00

Lowest Measured Frequency: 50.00

Result: Passed

Power Supply:

Averaging Period: 30.0

Datapoint Count: 20

	Lower Limit (V)	Actual (V)	Upper Limit (V)	Result:
12.00 V Rail	10.80	12.12	13.20	Passed
-12.00 V Rail	-13.20	-11.90	-10.80	Passed
5.00 V Rail	4.50	5.04	5.50	Passed
310.00 V Rail	279.00	320.00	341.00	Passed

เอกสารไม่ควบคุม

Optics

Beam Balance:

Lamp Type: Copper **Peak Selected:** 324.80

Lamp Socket Used: 3 **Lamp Alignment:** Performed

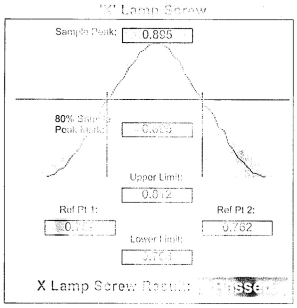

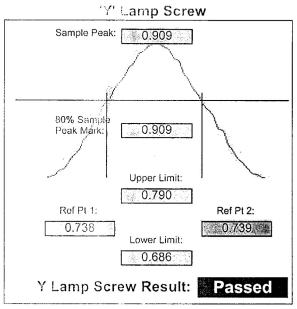

Grating S[illegible]:

Lamp Element(s): Copper

Lamp Turret Position: 3

Lamp Current(mA): 4.00

Slit Width(nm): 0.5

1st Order Wavelength(nm): 324.80

Lamp Alignment: [illegible]

	Lower Limit (nm)	Actual (nm)	Upper Limit (nm)	Result:
Zero Order	-0.10	0.00	0.10	Passed
First Order	324.45	324.75	325.15	Passed
Second Order	649.29	649.51	649.97	Passed

เอกสารไม่ควบคุม

Wavelength Repeatability:

Lamp Used: Copper
Lamp Current(mA): 4
Peak Used(nm): 324.750
Slit Width(nm): 0.2
Connected to Socket: 3
Slit Height: Normal

Lamp Alignment:

Lower Limit(nm) 324.788 324.888 Upper Limit(nm)

(Approach from Zero Order)	(Approach from end)
Sample 1: 324.823	Sample 2: 324.823
Sample 3: 324.823	Sample 4: 324.823
Sample 5: 324.823	Sample 6: 324.819
Sample 7: 324.819	Sample 8: 324.819
Sample 9: 324.823	Sample 10: 324.819

Mean: 324.822 Standard Deviation: 0.003

Result:

เอกสารไม่ควบคุม

Mechanical

Wavelength Drive:

Slit Drive:

Turret Drive:

Auto Burner Adjuster Drive:

Miscellaneous

Signal Processing Linearity:

Calculate Mode: New Calc Mode

	Lower Limit	Actual	Upper Limit	Result:
S5	194		297	Passed
S4	166	184	191	Passed
S3	271	316	332	Passed
S2	474	517	579	Passed
S1	826	913	1008	Passed
S0	1485	1618	1754	Passed
S-1	2498	2729	3053	Passed
S-2	4247	4613	5313	Passed

Interlocks:

Burner Fitted:
N2O Burner Fitted:
Flame Shield Closed:
Gas Control Fitted:
Pressure Release Bung Fitted:
Liquid Trap Closed:

Flame Detect: Working
GCU Active: Working
Oxidant Pressure: Working
Oxidant Changeover: Untested
Ignition: Working

เอกสารไม่ควบคุม

Auto Lamp Recognition:

Lamp 1: Uncoded Lamp/Not Connected
Lamp 2: 87 - Silver/Cadmium/Lead/Zinc(UltrAA) (Ag/C
Lamp 3: 14 - Copper (Cu)
Lamp 4: Uncoded Lamp/Not Connected
Lamp 5: Not Supported
Lamp 6: Not Supported
Lamp 7: Not Supported
Lamp 8: Not Supported

Result: Passed

GTA Temperature Monitoring:

Notes:

Signatures:

UAE	Date	Kanyakorn S.	30 Jan 2025
		Kanyakorn S.	Date

เอกสารไม่ควบคุม

Sequential by time report 1/30/2025 10:53 AM SpectrAA
Page 1 of 1

Analyst
Date Started 1/30/2025 10:33 AM GMT: 1/30/2025 3:33 AM
Worksheet Sensitivity Test 01
Comment
Methods Cu
Computer name DESKTOP-R9UIFRS
Serial Number: MY13160001

Method: Cu (Flame)

Sample ID	Conc mg/L	%RSD	Mean Abs		
CAL ZERO	0.000	38.8	0.0002		
	Readings				
	0.0002	0.0003	0.0001	1/30/2025	10:51:46 AM
STANDARD 1	5.000	0.1	0.5571		
	Readings				
	0.5574	0.5563	0.5575	1/30/2025	10:52:22 AM



Curve Fit = Linear Origin
Characteristic Conc = 0.039 mg/L
r = 1.0000
Calculated Conc = 0.002 5.000
Residuals = -0.002 0.000

Abs = 0.11141 x C

5 ppm Cu	5.025	0.3	0.5598		
	Readings				
	0.5582	0.5596	0.5615	1/30/2025	10:52:54 AM

เอกสารไม่ควบคุม

Sequential by time report 1/30/2025 10:48 AM SpectrAA
Page 1 of 1

Analyst
Date Started 1/30/2025 10:33 AM GMT: 1/30/2025 3:33 AM
Worksheet Precision Test
Comment
Methods Cu
Computer name DESKTOP-R9UIFRS
Serial Number: MY13160001

Method: Cu (Flame)

Sample ID	Conc mg/L	%RSD	Mean Abs		
CAL ZERO	0.000	64.1	-0.0002		
	Readings				
	-0.0003	-0.0003	-0.0001	1/30/2025	10:46:52 AM
STANDARD 1	5.000	0.3	0.6052		
	Readings				
	0.6036	0.6073	0.6047	1/30/2025	10:47:24 AM

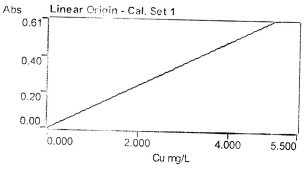

Curve Fit = Linear Origin
Characteristic Conc = 0.036 mg/L
r = 1.0000
Calculated Conc = -0.002 5.000
Residuals = 0.002 0.000

Abs = 0.12105 x C

5 ppm Cu	5.007	0.2	0.6061			
	Readings					
	0.6065	0.6052	0.6047	0.6047	0.6042	0.6079
	0.6055	0.6076	0.6064	0.6079	1/30/2025	10:48:32 AM

Flame Optimization

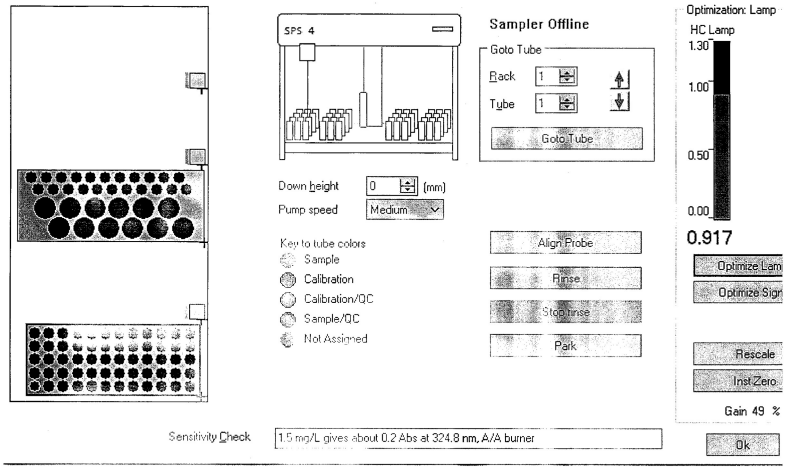

เอกสารไม่ควบคุม

เอกสารไม่ควบคุม

TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL.0-2717-3000-29 FAX.0-2719-9484

NSC-TISI-TIS17025 CALIBRATION 0008

Certificate of Calibration

Cert.No.: 25CH167
Page.: 1 of 3

Equipment :	Conductivity Meter
Manufacturer :	Horiba
Model :	LAQUA-EC210
Serial No. :	HC9L0013
ID No. :	UAE.EFM.011/2563(EFM.SCT.05/63)
Condition As-Received:	Used Item
Received Date :	04 February 2025
Calibration Date :	05 February 2025
Reference :	2502-0107WSC-3
Submitted by :	United Analyst and Engineering Consultant Co.,Ltd. 3 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Ambient Temperature :	(25 ± 2.5) °C
Relative Humidity :	(50 ± 15) %
Calibration Procedure:	In -house method : - CP-CH6 by direct measurement with certified reference material (CRM) - CP-CH8 by comparison with temperature standard
Calibrated by :	Warakorn Lerngagtrakul
Approved by :	Approved Signatory

( ) Chakrit Waewwanjua
( ) Ponpan Paipim
(✓) Saithip Meangmai

Issue Date : 06 February 2025

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

Condition of this result of calibration

1. Reference Standard Instrument :-

Instrument	Serial No.	ID No.	Certificate No.	Due date
1) Thermometer	1963878	130RC095	24I995	09 Sep 2025
2) Ref. Std.Thermometer	4982054	110RC044	24I757	14 July 2025

- This Certification is traceable to SI Throught Technology Promotion Association (Thailand - Japan)

2. Certified Reference Materials :-
- Conductivity calibration solution, CPA chem Ltd., The measurement results are traceable to SI through CPA chem Ltd., ANSI-ASQ National Accreditation Board, Accredited No. AR-1835

Conductivity Solution	Manufacturer	Lot No.	Exp. date
1412.9 µS/cm	CPA Chem	1005307	15 June 2025
12.881 mS/cm	CPA Chem	1005308	15 June 2025

- Control Conductivity calibration solution temperature by Water bath (25 ± 0.1) °C

3. This certificate is valid only to the item calibrated on date and place of calibration.

Calibration results

Function : Conductivity Measurement
(*) After Adjustment at 1412.9 µS/cm
Conductivity Electrode Serial No.: 9B9F0286

Standard Conductivity Solution	Before Adjustment UUC* Reading	After Adjustment UUC* Reading	Uncertainty of Measurement (±)	Coverage factor *k*
1412.9 µS/cm	1444 µS/cm	1413 µS/cm	9.2 µS/cm	2.00
12.881 mS/cm	12.94 mS/cm	12.66 mS/cm	0.086 mS/cm	2.00

Remark : - UUC* = Unit Under Calibration

Calibration Results

Function : Temperature Measurement

This equipment was connected with Temperature Probe;

- Model : 9383
- Serial No. : 9B9F0286

Dimension of probe;

- Length : 110 mm
- Diameter : 16 mm
- Immersion Depth : 100 mm

Calibration Result : Without adjustment

Calibration Point (°C)	Standard Temperature (°C)	UUC* Reading (°C)	Error (°C)	Uncertainty of Measurement (± °C)	Coverage factor *k*
15.0	15.003	15.0	-0.003	0.13	2.00
30.0	30.004	30.0	-0.004	0.13	2.00
45.0	45.003	45.0	-0.003	0.13	2.00

Remark : - UUC* = Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

SCIENCE TECH CO., LTD.
Head Office : 321/43 Nanglinchee Rd. Chongnondsee Yannawa Bangkok 10210 Thailand Tel. 0-2285-4101 Fax. 0-2285-4856 www.sciencetech.th.com
Science Tech Laboratory : 279/27-29 Soi Watpoman Sathupradit 19 Rd. Chongnondsee Yannawa Bangkok 10120 Tel. 0-2285-4101 Fax. 0-2285-4856

NSC-TISI-TIS 17025 CALIBRATION 0402

Job No. : J014/25 **Certificate No. : ST014/25**

Certificate of Calibration

Equipment : pH/ISE Meter
Manufacturer : Orion
Made in : USA
Model : STAR A214
Serial No. : X36836
ID No. : UAE.WAT.025/2560
Range : 0 to 14 pH
Resolution : 0.001 pH 0.1 mV
UUC Condition As-Received : Good
Submitted by : บริษัท ยูไนเต็ด แอนนาลิสต์ แอนด์ เอ็นจิเนียริ่ง คอนซัลแตนท์ จำกัด 3 ซอยอุดมสุข 41 ถนนสุขุมวิท แขวงบางจาก เขตพระโขนง กรุงเทพฯ 10260
Ambient Temperature : (25 ± 3) °C
Relative Humidity : (50 ± 15)%
Calibration Procedure : In - house method : WI-ST-LAB-7.2/I based on direct measurement by using standard voltage calibrator
Issue date : Wednesday, May 21, 2025

Calibrateded by : Khannika Sangkham **Approved by :**

(Khannika Sangkham)
Laboratory manager

The uncertainties are for a confidence probability of approximately 95%

This certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other **than in full, except with the prior written approval of the Science Tech Laboratory.**

เอกสารไม่ควบคุม

Certificate of Calibration

Job No. : J014/25 **Certificate No. : ST014/25**

Received date : Friday, May 16, 2025

Calibration date : Tuesday, May 20, 2025

Condition of this calibration result

1 Reference standard instrument : Voltage calibrator Yokogawa 7651 S/N. 91H441999 Certificate No. 24E3876
Due date 12 June 2025 TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)

2 This certificate was certified only for the instrument we calibrated

3 This result of calibration was found accurate as shown on date and place of calibration only

Result of Calibration

Function : pH meter

Performing standard curve by Voltage Calibrator at pH (4,7,10)

Unit Under Calibration	Applied Voltage (mV)	Nominal Value (pH)	UUC Reading (mV)	Correction (mV)	Uncertainty (± mV)	k Factor
pH Meter	177.48	4	177.4	0.1	0.060	2.00
Model STAR A214	0.0	7	0.0	0.0	0.064	2.00
S/N. X36836	-177.48	10	-177.4	-0.1	0.078	2.00

This reported uncertainty of measurment was based on a standard uncertainty multiplied by a coverage factor k , providing a level of confidence of approximately 95%

-oooo- End of Certificate of Calibration -oooo-

เอกสารไม่ควบคุม

SCIENCE TECH CO., LTD.
Head Office : 321/43 Nanglinchee Rd. Chongnondsee Yannawa Bangkok 10120 Thailand Tel. 0-2285-4101 Fax. 0-2285-4856 www.sciencetech.th.com
Science Tech Laboratory : 279/27-29 Soi Watpoman Sathupradit 19 Rd. Chongnondsee Yannawa Bangkok 10120 Tel. 0-2285-4101 Fax. 0-2285-4856

Job No. : JF006/25 **Certificate No. : FT006/25**

Certificate of Calibration

Equipment : pH/ISE Meter
Manufacturer : Orion
Made in : USA.
Model : STAR A214
Serial No. : X36836
ID No. : UAE.WAT.025/2560
Ion Selective Model : 9409BN
Serial No. : ZW1-18420
Referance Electrode Model : 900100
Serial No. : ZW1-16834
Range : 0 to 14 pH
Resolution : 0.001 pH 0.1 mV
Submitted by : บริษัท ยูไนเต็ด แอนนาลิสต์ แอนด์ เอ็นจิเนียริ่ง คอนซัลแตนท์ จำกัด 3 ซอยอุดมสุข 41 ถนนสุขุมวิท แขวงบางจาก เขตพระโขนง กรุงเทพฯ 10260
Ambient Temperature : (25 ± 3) °C
Relative Humidity : (50 ± 15)%
Issue date : Wednesday, May 21, 2025

Calibrateded by : Khannika Sangkham

Approved by :

(Khannika Sangkham)
Laboratory manager

เอกสารไม่ควบคุม

Certificate of Calibration

Job No. : JF006/25 **Certificate No. :** FT006/25

Received date : Friday, May 16, 2025 **Page :** 2 of 2

Calibration date : Tuesday, May 20, 2025

Condition of this calibration result

1 Reference standard materials : Certified Fluoride standard reference solution (Directly measured by differential potentiometry with the aid of potassium fluoride "quasi without transference" against solutions prepared from primary reference materials from NIST)

2 This certificate was certified only for the instrument we calibrated

3 This result of calibration was found accurate as shown on date and place of calibration only

Result of Calibration

Function : pH/ISE Meter with Probe

Direct Measurement

First Standard concentrated	=	0.1	ppm
Secondary Standard concentrated	=	1	ppm
Tertiary Standard concentrated	=	10	ppm
Fourthly Standard concentrated	=	100	ppm
Slope	=	**-58.4**	mV/Dec.

Channel : 1

Unit Under Calibration	Standard Concentrated (ppm)	UUC Reading (ppm)	Correction (ppm)	Stdev (ppm)
Model :	0.1	0.109	-0.009	0.00
9409BN S/N. ZW1-18420	1	1.03	-0.02	0.01
900100 S/N. ZW1-16834	10	9.97	0.03	0.03
	100	99.6	0.4	1.17

-oo0oo-

เอกสารไม่ควบคุม

FOSS

FOSS South East Asia
3388 Sirinrat Building, 25th – 26th Floor, Unit No. 3388/90,
Rama IV Road, Klongton , Klongtoey, Bangkok, Thailand 10110

Customer Service Report

Report No.: 13319

Date: Jan 27, 2025 **Customer:** UAE

Job No.: 11675 **Address:** Bangkok

Instrument: KT200 **Serial:** 91790524

	Travel To Customer (Hrs)		Labour (Hrs)		Travel From Customer (Hrs)	
Start	09.00	1	10.00	3	-	-
Finish	10.00		13.00		-	

Job Type

Application		Special		Standard			
Distributor	x	Courtesy Visit	x	Installation	x	Training	x
Digital Service	x	PMA Onboarding	x	Quote	x	In House	
Internal	x	Warranty	x	Repair	x	PM	x
Investigate	x	Sales Support	x	Remote	x	Health Check Visit	x

PMA Type					
	Smartcare	x	Smartcare Pro		Fosscare
	Smartcare Advance		Fosscare Pro		N/A

Details of Work / Test

- PM -
+ Visual Check +
- No leak - ok
- have damage on heater & main switch - not ok
+ Clean heater 110° main Switch Explosion Vial - ok
+ Clean PM kit * 1 set - ok
+ Function Check
- Power on/OFF
- Alkali
- Steam
- Condenser
water pump - ok

Instrument Ready for Use OK x Not OK* x

Part No:	Batch	Description	Qty
100 09965	11.06.2024	FOSS PM kit KT200 &Better Analyser/2100	1
10003572	29.03.2024	Heating element Steam	1
15630111	19.10.2022	Switch R595KMT+2 FR	1

I confirm this report is accurate and complete

Signed FOSS		Signed Customer	
Name		Name	

Email: Customer Contact.:

*Remark:

เอกสารไม่ควบคุม

FOSS

FOSS South East Asia
3388 Sirinrat Building, 25th – 26th Floor, Unit No. 3388/90,
Rama IV Road, Klongton , Klongtoey, Bangkok, Thailand 10110

Customer Service Report

Report No.: 13854

Date: 24 February 2025 **Customer:** UAE

Job No.: 11735 **Address:** BANGKOK

Instrument: KT810U **Serial:** 91889052

	Travel To Customer (Hrs)		Labour (Hrs)		Travel From Customer (Hrs)	
Start	07:00	2hrs	09:00-12:00	3hrs	15:00	
Finish	09:00		13:00-14:00		17:00	

Job Type

Application		Special		Standard			
Distributor	x	Courtesy Visit	x	Installation	x	Training	
Digital Service	x	PMA Onboarding	x	Quote	x	In House	
Internal	x	Warranty	x	Repair	x	PM	x
Investigate	x	Sales Support	x	Remote	x	Health Check Visit	x

PMA Type					
	Smartcare	x	Smartcare Pro		Fosscare
	Smartcare Advance	x	Fosscare Pro		N/A

Details of Work / Test

PM KT800 12mo

- test before pm
- Cleaning KT800, 36 mo replace
- fushing Alkali pump
- test operation
  - Distan 80 - 80 mL
  - Distillation 6 min 150 - 170 mL
  - Alkali 50 - 80 mL
  - All pass

Instrument Ready for Use OK x Not OK* x

Part No:	Batch	Description	Qty
60031810	08.01.2024	FOSS PM kit KT800 &200 36mo	1

I confirm this report is accurate and complete

Signed FOSS		Signed Customer	Supharkorn P.
Name		Name	

Email: Customer Contact.:

*Remark:

Please scan QR code

เอกสารไม่ควบคุม

DQE Services Co.,Ltd.
32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Ladprao, Bangkok 10230
Phone : +66 (0)2 538 2054, Email : dqeservicesinfo@gmail.com

NSC-TISI-TIS 17025 CALIBRATION 0404

CERTIFICATE OF CALIBRATION

Certificate No. : SP25-019 Page 1 of 5

Customer : United Analyst and Engineering Consultant Co.,Ltd. (Head Office)

Address : 3 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260

Location of calibration : Instrument room (207)

Equipment : UV-Vis Spectrophotometer

Manufacturer : Agilent Technologies

Model : Cary 60

Serial No. : MY15410009

ID No. : UAE.WAT.020/2558

Received Date : 26 May 2025

Calibration Date : 26 May 2025

Issue Date : 29 May 2025

Condition Instrument : Good

Calibrated by : (Mr.Tanawut Rittidach) Technical Manager

Approved by : (Ms.Chonticha Sangngern) Quality Manager

The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only.

The measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the DQE Services Co., Ltd.

เอกสารไม่ควบคุม

FM-708-02 R01 1/11/2021

DQE Services Co.,Ltd.
32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Ladprao, Bangkok 10230
Phone : +66 (0)2 538 2054, Email : dqeservicesinfo@gmail.com

NSC-TISI-TIS 17025 CALIBRATION 0404

REPORT OF CALIBRATION

Certificate No. : SP25-019

Environment Condition : Ambient Temperature 25 ± 5 °C

Relative humidity 55 ± 20 %RH

Calibration method : In-house method CP-01 Based on ASTM E275-08

Certified Reference Materials :

Material	Serial No.	Certificate No.	Due date
Absobance Standard set	25760	115663	25 October 2025
Absobance Standard set	25757	115638	25 October 2025
Wavelength Standard set	25806	115657	25 October 2025
Wavelength Standard set	25758	115665	25 October 2025

Traceability : This certification is traceable to the International System of Unit maintained at National - Institute of Standards and Technology (NIST) through Starna Scientific Limited

Spectral Band Width of UUC : 1.5 nm.

Scan Speed of UUC : 60 nm/min

Scan Interval of UUC : 0.15 nm.

Resolution of UUC : Photometric 0.0001 Abs.

Wavelength 0.1 nm.

เอกสารไม่ควบคุม

DQE Services Co.,Ltd.
32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Ladprao, Bangkok 10230
Phone : +66 (0)2 538 2054, Email : dqeservicesinfo@gmail.com

NSC-TISI-TIS 17025 CALIBRATION 0404

REPORT OF CALIBRATION

Certificate No. : SP25-019

Calibration Results : Without adjustment

Photometric Accuracy :

Wavelength (nm.)	CRMs Values (Abs)	UUC Reading (Abs)	Correction (Abs)	Uncertainty (Abs)	Coverage factor *k*
420	0.0000	0.0000	0.0000	0.0028	2.00
	0.5780	0.5739	0.0041	0.0031	2.00
	1.0484	1.0430	0.0054	0.0029	2.00
	2.1876	2.1876	0.0000	0.0084	2.00
440	0.0000	0.0000	0.0000	0.0028	2.00
	0.5595	0.5581	0.0014	0.0034	2.00
	1.0239	1.0219	0.0020	0.0035	2.00
	2.1230	2.1207	0.0023	0.0085	2.00
465	0.0000	0.0000	0.0000	0.0028	2.00
	0.5230	0.5190	0.0040	0.0029	2.00
	0.9633	0.9609	0.0024	0.0029	2.00
	1.9753	1.9719	0.0034	0.0079	2.00
546.1	0.0000	0.0000	0.0000	0.0028	2.00
	0.5181	0.5161	0.0020	0.0031	2.00
	1.0002	0.9979	0.0023	0.0033	2.00
	1.9973	2.0021	-0.0048	0.0102	2.00
590	0.0000	0.0000	0.0000	0.0028	2.00
	0.5517	0.5503	0.0014	0.0030	2.00
	1.0803	1.0808	-0.0005	0.0031	2.00
	2.0373	2.0324	0.0049	0.0105	2.00
635	0.0000	0.0000	0.0000	0.0028	2.00
	0.5591	0.5583	0.0008	0.0031	2.00
	1.0518	1.0513	0.0005	0.0030	2.00
	1.9274	1.9281	-0.0007	0.0102	2.00

เอกสารไม่ควบคุม

FM-708-02 R01 1/11/2021

DQE Services Co.,Ltd.
32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Ladprao, Bangkok 10230
Phone : +66 (0)2 538 2054, Email : dqeservicesinfo@gmail.com

NSC-TISI-TIS 17025 CALIBRATION 0404

REPORT OF CALIBRATION

Certificate No. : SP25-019

Photometric Accuracy :

Wavelength (nm.)	CRMs Values (Abs)	UUC Reading (Abs)	Correction (Abs)	Uncertainty (Abs)	Coverage factor *k*
235	0.0000	0.0000	0.0000	0.0050	2.00
	0.7469	0.7488	-0.0019	0.0063	2.00
257	0.0000	0.0000	0.0000	0.0050	2.00
	0.8674	0.8663	0.0011	0.0067	2.00
313	0.0000	0.0000	0.0000	0.0050	2.00
	0.2919	0.2902	0.0017	0.0052	2.00
350	0.0000	0.0000	0.0000	0.0050	2.00
	0.6430	0.6428	0.0002	0.0063	2.00

เอกสารไม่ควบคุม

FM-708-02 R01 1/11/2021

DQE Services Co.,Ltd.
32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Ladprao, Bangkok 10230
Phone : +66 (0)2 538 2054, Email : dqeservicesinfo@gmail.com

NSC-TISI-TIS 17025 CALIBRATION 0404

REPORT OF CALIBRATION

Certificate No. : SP25-019

Wavelength Accuracy :

CRMs Values (nm.)	UUC Reading (nm.)	Correction (nm.)	Uncertainty (nm.)	Coverage factor *k*
241.72	242.0	-0.28	0.18	2.00
279.45	279.5	-0.05	0.18	2.00
287.81	287.6	0.21	0.18	2.00
334.06	333.8	0.26	0.18	2.00
360.93	360.5	0.43	0.18	2.00
418.59	417.9	0.69	0.18	2.00
445.94	445.4	0.54	0.18	2.00
453.66	453.2	0.46	0.18	2.00
460.02	459.6	0.42	0.18	2.00
536.59	536.5	0.09	0.18	2.00
637.98	638.5	-0.52	0.18	2.00
431.38	430.7	0.68	0.18	2.00
472.50	472.3	0.20	0.18	2.00
513.47	513.5	-0.03	0.18	2.00
528.88	528.9	-0.02	0.18	2.00
573.17	573.8	-0.63	0.18	2.00
585.35	585.2	0.15	0.20	2.00
684.40	685.1	-0.70	0.18	2.00
740.72	741.1	-0.38	0.20	2.00
748.55	748.9	-0.35	0.18	2.00
807.03	807.1	-0.07	0.18	2.00
879.28	879.1	0.18	0.18	2.00

Remark : - UUC = Unit Under Calinration

- N/A = Not Avaiable

- The result expanded uncertainty of measurement U is stated as the standard uncertainty of measurement multiplied by the coverage factor *k* , which for a normal distribution corresponds to a coverage probability of approximately 95%

- End of Certificate -

เอกสารไม่ควบคุม

FM-708-02 R01 1/11/2021

DQE Services Co.,Ltd.
32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Ladprao, Bangkok 10230
Phone : +66 (0)2 538 2054, Email : dqeservicesinfo@gmail.com

NSC-TISI-TIS 17025 CALIBRATION 0404

CERTIFICATE OF CALIBRATION

Certificate No. : SP25-021

Customer : United Analyst and Engineering Consultant Co.,Ltd. (Head Office)

Address : 3 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260

Location of calibration : Instrument room (207)

Equipment : UV-Vis Spectrophotometer

Manufacturer : HITACHI

Model : U-2900

Serial No. : 21E22-009

ID No. : UAE.WAT.051/2564

Received Date : 26 May 2025

Calibration Date : 26 May 2025

Issue Date : 29 May 2025

Condition Instrument : Good

Calibrated by : ปนงส
(Mr.Tanawut Rittidach)
Technical Manager

Approved by : ชลธิชา
(Ms.Chonticha Sangngern)
Quality Manager

The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only.

The measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the DQE Services Co., Ltd.

เอกสารไม่ควบคุม

DQE Services Co.,Ltd.
32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Ladprao, Bangkok 10230
Phone : +66 (0)2 538 2054, Email : dqeservicesinfo@gmail.com

NSC-TISI-TIS 17025 CALIBRATION 0404

REPORT OF CALIBRATION

Certificate No. : SP25-021

Environment Condition : Ambient Temperature 25 ± 5 °C

Relative humidity 55 ± 20 %RH

Calibration method : In-house method CP-01 Based on ASTM E275-08

Certified Reference Materials :

Material	Serial No.	Certificate No.	Due date
Absobance Standard set	25760	115663	25 October 2025
Absobance Standard set	25757	115638	25 October 2025
Wavelength Standard set	25806	115657	25 October 2025
Wavelength Standard set	25758	115665	25 October 2025

Traceability : This certification is traceable to the International System of Unit maintained at National - Institute of Standards and Technology (NIST) through Starna Scientific Limited

Spectral Band Width of UUC : 1.5 nm.

Scan Speed of UUC : 200 nm/min

Scan Interval of UUC : 0.1 nm.

Resolution of UUC : Photometric 0.001 Abs.

Wavelength 0.1 nm.

เอกสารไม่ควบคุม

DQE Services Co.,Ltd.
32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Ladprao, Bangkok 10230
Phone : +66 (0)2 538 2054, Email : dqeservicesinfo@gmail.com

NSC-TISI-TIS 17025 CALIBRATION 0404

REPORT OF CALIBRATION

Certificate No. : SP25-021

Calibration Results : Without adjustment

Photometric Accuracy :

Wavelength (nm.)	CRMs Values (Abs)	UUC Reading (Abs)	Correction (Abs)	Uncertainty (Abs)	Coverage factor *k*
420	0.0000	0.000	0.0000	0.0028	2.00
	0.5780	0.574	0.0040	0.0031	2.00
	1.0484	1.043	0.0054	0.0029	2.00
	2.1876	2.185	0.0026	0.0075	2.00
440	0.0000	0.000	0.0000	0.0028	2.00
	0.5595	0.558	0.0015	0.0034	2.00
	1.0239	1.022	0.0019	0.0035	2.00
	2.1230	2.121	0.0020	0.0079	2.00
465	0.0000	0.000	0.0000	0.0028	2.00
	0.5230	0.519	0.0040	0.0030	2.00
	0.9633	0.960	0.0033	0.0029	2.00
	1.9753	1.973	0.0023	0.0070	2.00
546.1	0.0000	0.000	0.0000	0.0028	2.00
	0.5181	0.516	0.0021	0.0031	2.00
	1.0002	0.998	0.0022	0.0033	2.00
	1.9973	1.995	0.0023	0.0084	2.00
590	0.0000	0.000	0.0000	0.0028	2.00
	0.5517	0.550	0.0017	0.0030	2.00
	1.0803	1.080	0.0003	0.0030	2.00
	2.0373	2.036	0.0013	0.0079	2.00
635	0.0000	0.000	0.0000	0.0028	2.00
	0.5591	0.558	0.0011	0.0031	2.00
	1.0518	1.051	0.0008	0.0030	2.00
	1.9274	1.926	0.0014	0.0079	2.00

เอกสารไม่ควบคุม

DQE Services Co.,Ltd.
32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Ladprao, Bangkok 10230
Phone : +66 (0)2 538 2054, Email : dqeservicesinfo@gmail.com

NSC-TISI-TIS 17025 CALIBRATION 0404

REPORT OF CALIBRATION

Certificate No. : SP25-021

Photometric Accuracy :

Wavelength (nm.)	CRMs Values (Abs)	UUC Reading (Abs)	Correction (Abs)	Uncertainty (Abs)	Coverage factor *k*
235	0.0000	0.000	0.0000	0.0050	2.00
	0.7469	0.748	-0.0011	0.0057	2.00
257	0.0000	0.000	0.0000	0.0050	2.00
	0.8674	0.866	0.0014	0.0059	2.00
313	0.0000	0.000	0.0000	0.0050	2.00
	0.2919	0.291	0.0009	0.0051	2.00
350	0.0000	0.000	0.0000	0.0050	2.00
	0.6430	0.640	0.0030	0.0055	2.00

เอกสารไม่ควบคุม

DQE Services Co.,Ltd.
32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Ladprao, Bangkok 10230
Phone : +66 (0)2 538 2054, Email : dqeservicesinfo@gmail.com

NBC-TISI-TIS 17025
CALIBRATION 0404

REPORT OF CALIBRATION

Certificate No. : SP25-021

Wavelength Accuracy :

CRMs Values (nm.)	UUC Reading (nm.)	Correction (nm.)	Uncertainty (nm.)	Coverage factor *k*
241.72	241.0	0.72	0.18	2.00
279.45	278.8	0.65	0.18	2.00
287.81	287.2	0.61	0.18	2.00
334.06	333.6	0.46	0.18	2.00
360.93	360.6	0.33	0.18	2.00
418.59	418.2	0.39	0.18	2.00
445.94	445.6	0.34	0.18	2.00
460.02	459.8	0.22	0.18	2.00
536.59	536.6	-0.01	0.18	2.00
637.98	638.0	-0.02	0.18	2.00
431.38	431.2	0.18	0.18	2.00
472.50	472.4	0.10	0.18	2.00
513.47	513.4	0.07	0.18	2.00
528.88	528.8	0.08	0.18	2.00
573.17	573.2	-0.03	0.18	2.00
585.35	585.0	0.35	0.20	2.00
684.40	684.4	0.00	0.18	2.00
740.72	741.0	-0.28	0.20	2.00
748.55	748.8	-0.25	0.18	2.00
807.03	807.2	-0.17	0.18	2.00
879.28	879.6	-0.32	0.18	2.00

Remark : - UUC = Unit Under Calinration

- N/A = Not Avaiable
- The result expanded uncertainty of measurement U is stated as the standard uncertainty of measurement multiplied by the coverage factor *k* , which for a normal distribution corresponds to a coverage probability of approximately 95%

- End of Certificate -

เอกสารไม่ควบคุม