



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES

534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL.0-2717-3000-29 FAX.0-2719-9484

Certificate of Calibration

Cert.No.: 25CH218

Page.: 1 of 2

Equipment :	pH Meter
Manufacturer :	Waterproof
Model :	pHTestr 30
Serial No. :	3195382
ID No. :	-
Condition As-Received:	Used Item
Received Date :	18 February 2025
Calibration Date :	19 February 2025
Reference :	2502-0526DN-3
Submitted by :	Environment Research & Technology Company Limited. 25/114 Moo 6, Soi Chinaket 1, Ngamwongwan Road, Toongsonghong, Laksi, Bangkok 10210
Ambient Temperature :	(25 ± 2.5) °C
Relative Humidity :	(50 ± 15) %
Calibration Procedure :	In - house method : - CP-CH5 by direct measurement with reference material (RM)

Calibrated by :

Approved by :

19 February 2025

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Calibration and Testing Equipment Services.



Cert.No.: 25CH218

Page.: 2 of 2

Condition of this calibration result

1. Certified Reference Materials : Standard buffer solution (Traceable to NIST, U.S.A.)

<u>Buffer Solution</u>	<u>Manufacturer</u>	<u>Lot No.</u>	<u>Exp. date</u>
pH 4.01	Thermo Scientific	403/03	06 Oct 2026
pH 7.00	Thermo Scientific	402/01	07 Oct 2025
pH 10.01	Thermo Scientific	363/03	08 Sep 2026

2. This certificate is valid only to the item calibrated on date and place of calibration.

Calibration Results

Function : pH Measurement

Performing three buffers standard curve by using buffer nominal pH (4,7,10)

Unit Under Calibration	Standard pH Buffer Solution	Actual pH Reading	Actual mV Reading (mV)	Uncertainty of pH Measurement ($\pm$)	Coverage factor k
pH Electrode S/N.: 3195382	4.01	4.01	N/A	0.012	2.00
	7.00	7.00	N/A	0.013	2.00
	10.01	10.01	N/A	0.016	2.00

Remark

- pH meter does not have voltage mode.
- Can not connect the BNC because the plug does not match with the socket.
- N/A = Not Available

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k , providing a level of confidence of approximately 95 %.

-o0o-



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3 : EQUIPMENT CALIBRATION AND TESTING SERVICES


534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250

TEL. 0-2717-3000 FAX. 0-2719-9484

Certificate of Testing

Cert.No.: 24TW185

Page.: 1 of 2

Equipment : DO Meter
Manufacturer : YSI
Model : 5000-115V
Serial No. : 03C1280 AC
ID No. : ERTC-L-In-164
Received Date : 03 September 2024
Test Date : 04 September 2024
Reference : 2409-0126DN-1
Submitted by : Environment Research & Technology Company Limited.
25/114 Moo 6, Soi Chinaket 1, Ngamwongwan Road,
Toongsonghong, Laksi, Bangkok 10210
Laboratory Condition : Temperature (25 ± 5) °C
Humidity (50 ± 20) %
Test Procedure : In - house method : CP-CH9
by Comparison Technique with Azide Modification Method
Tested by : 
Approved by : 
Issue Date : 6 September 2024



Cert.No.: 24TW185

Page.: 2 of 2

Condition of this result of calibration

1. Reference Standard Instruments :

This certification is traceable to the International System of Unit through the reference standards laboratory of Industrial Calibration Center, Technology Promotion Association (Thailand-Japan).

<u>Instruments</u>	<u>Serial No.</u>	<u>ID No.</u>	<u>Certificate No.</u>	<u>Due Date</u>
1. Burette	-	130BU10	23CG1172	22 Mar 2025
2. Balance	N03679	140RC001	23MM537	14 Sep 2024

2. Standard Material :-

<u>Material</u>	<u>Manufacturer</u>	<u>Lot.No.</u>	<u>Assay</u>
Sodium Thiosulfate 5-Hydrate AR	KEMAUS	2203162447	99.6%

Result : **Dissolved Oxygen Meter Adjustment With Air 100 %**

Dissolved Oxygen Probe No.: 15K100353

Titration Method (Azide Modification Method) (mg/L)	DO Meter Reading (mg/L)	Standard Deviation (mg/L)
8.18	8.18	0.0055

This report was certified only for the instrument we tested. It is allowable to use for study
Intend to use for advertising and referral purpose is prohibited. This report may not be reproduced
other in full, without written approval of the laboratory

-o0o-



Inctech Metrological Center Co.Ltd.

39/1 Soi 82, Sukhapiban 5 Rd., O ngoen,

Saimai, Bangkok 10220, Thailand

Tel. (662) 909-8820 (Auto 10 lines) www.imcinstrument.com



Calibration Cert. # 3884.01
ISO/IEC 17025

Certificate of Calibration

Certificate No. : MT24-9500

Page : 1 of 2

Customer : Environment research & Technogy Co.,Ltd.

Address : 25/114 Moo6 Soi Chinaket1, Ngamwongwan Road, Toongsonghong, Laksi, Bangkok 10210

Description : Incubator

Manufacturer : Hotpack

Model : 352601

Serial No. : 78633

Identification No. : ERTC-L-In-133

Calibration Place : Customer Laboratory

Order No. : 4090/24

Received date : Nov 29, 2024

Calibration date : Nov 29, 2024

Environment Condition :

Temperature : (25+/-10) °C

Humidity : (50+/-30) %RH

Calibration Method : Calibration were conducted using In-house calibration procedure *CP-MT-006* According to comparison with LXI Data Acquisition Switch Unit with sensor. The calibration methods based on Euramet Calibration Guide No.20 - guidelines on the Calibration of Temperature and/or Humidity Controlled Enclosures.

Reference Standard Instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Certificate No.</u>	<u>Due Date</u>
Data Acquisition System with Sensor	DAQ970A	MY58003374	MT24-1056	Jan 05, 2025

The effect that the result relate only to the items calibrated. It was found accurate as shown on date and place of calibration only.

Traceability : This measurement are traceable to the International System of Unit (SI), through National Institute of Metrology Thailand (NIMT)

The reported expanded uncertainty of measurement was based on standard providing a level of confidence of not less than 95%

Calibrated by :



This calibration certificate shall not be reproduced other than in full except with the prior written approval of Inctech Metrological Center Co.,Ltd

**Inctech Metrological Center Co.Ltd.**

39/1 Soi 82, Sukhapiban 5 Rd., O ngoen,


Saimai, Bangkok 10220, Thailand

Tel. (662) 909-8820 (Auto 10 lines) www.imcinstrument.com

Calibration Cert. # 3884.01
ISO/IEC 17025**Certificate No. :** MT24-9500**Page :** 2 of 2**Function** : Temperature measurement**Calibration point** : 20 °C**Result** : Without adjustment**Resolution** : 0.1 °C

Calibration point (°C)	Temperature of UUC* at each position (°C)									Uncertainty of measurement (+/- °C)
	Ch.1	Ch.2	Ch.3	Ch.4	Ch.5	Ch.6	Ch.7	Ch.8	Ch.9	
20	20.276	20.230	20.142	20.019	19.785	20.414	20.187	20.072	20.426	0.41

Setting temperature (°C)	Indicating Temperature (°C)	Measured stability (+/- °C)	Measured uniformity (°C)	Overall variation (°C)
20.0	20.0	0.27	0.97	1.1

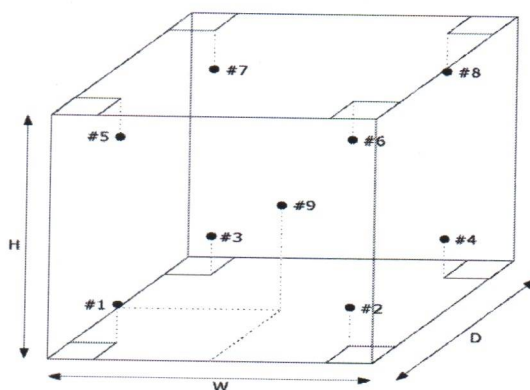**Front view**

- #1 Lower Left Front
- #2 Lower Right Front
- #3 Lower Left Rear
- #4 Lower Right Rear
- #5 Upper Left Front
- #6 Upper Right Front
- #7 Upper Left Rear
- #8 Upper Right Rear
- #9 Geometric Center

UUC* = Unit under calibration**Uniformity** = Maximum and Minimum difference of measured temperature at any probes and the measured temperature at the reference and same time.**Overall Variation** = Difference of temperature value between the maximum and minimum any time.**Stability** = One half of the maximum difference of measured temperatures at any one probe.

Mettler-Toledo (Thailand) Ltd.

846/4 - 846/5 Lasalle Rd., Bangna Tai Sub-District

Bangna District, Bangkok 10260

+662 723 0382

MT-TH.ServiceSupport@mt.com



NSC-TISI-TIS 17025
CALIBRATION 0062

Accuracy Calibration Certificate

Customer

Company: Environment Research & Technology
Address: 25/114 Moo 6, Soi Chinaket 1, Ngamwongwan Rd., Toongsonghong
City: Laksi **Contact:** Ramita Taengthai
Zip / Postal: 10210
State / Province: Bangkok
Order Number: 
0 3 3 3 6 1 0 1 9

Weighing Device

Manufacturer: Mettler Toledo **Instrument Type:** Weighing Instrument
Model: MS204S/01 **Asset Number:** ERTC-L-IN-088
Serial No.: B334691537 **Terminal Model:** N/A
Building: N/A **Terminal Serial No.:** N/A
Floor: 5 **Terminal Asset No.:** N/A
Room: 504

Range	Max. Capacity	Readability (d)
1	220 g	0.0001 g

Procedure

Calibration Guideline: EURAMET cg-18 v. 4.0/CENAM-ema:2015
METTLER TOLEDO Work Instruction: CP/W002/20


This calibration certificate contains measurements for As Found calibration. No As Left calibration was performed because the device was not modified after As Found calibration. Therefore, results for As Left correspond to As Found.

The sensitivity/span of the weighing instrument was adjusted before calibration with a built-in weight.

In accordance with EURAMET cg-18 (11/2015), the test loads were selected to reflect the specific use of the weighing device or to accommodate specific calibration conditions.

	Temperature		Humidity	
As Found	Start: 19.7 °C	End: 19.6 °C	Start: 40.0 %	End: 45.0 %

As Found Calibration Date: 15-Jan-2025
As Left Calibration Date: N/A
Issue Date: 17-Jan-2025

Calibrator: 
Approved Signatory: Technical Manager / Head of Calibration Center

Measurement Results


Repeatability

Test Load: 100 g

	As Found	As Left
1	100.0000 g	N/A
2	100.0001 g	N/A
3	100.0002 g	N/A
4	100.0001 g	N/A
5	100.0000 g	N/A
6	100.0001 g	N/A
7	100.0001 g	N/A
8	100.0000 g	N/A
9	100.0001 g	N/A
10	100.0001 g	N/A

Standard Deviation	0.00006 g	N/A
--------------------	-----------	-----

○ As Found
◆ As Left

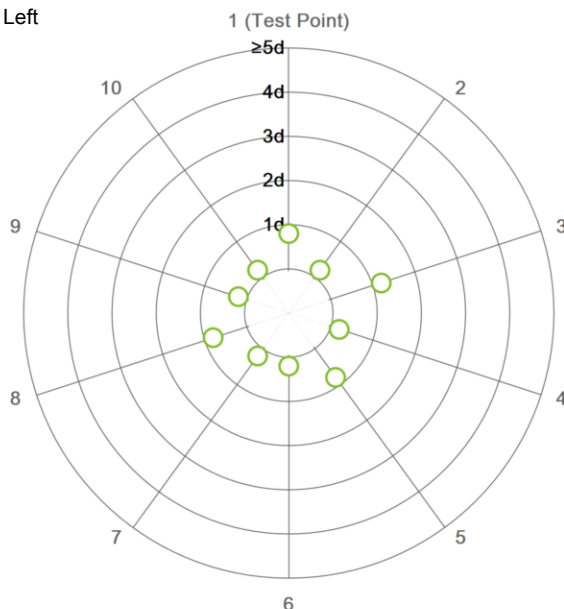

The "d" in the graph represents the readability of the range/interval in which the test was performed.


The results of this graph are based upon the absolute values of the differences from the mean value.

Eccentricity

Test Load: 100 g

Position	As Found	As Left
1	100.0000 g	N/A
2	100.0000 g	N/A
3	99.9999 g	N/A
4	100.0000 g	N/A
5	100.0001 g	N/A

Maximum Deviation	0.0001 g	N/A
-------------------	----------	-----




As Found

The "d" in the graph represents the readability of the range/interval in which the test was performed.

Error of Indication

As Found

	Reference Value	Indication	Error of Indication	Expanded Uncertainty	k
1	0.0000 g	0.0000 g	0.0000 g	0.14 mg	2
2	0.0500 g	0.0500 g	0.0000 g	0.15 mg	2
3	0.1000 g	0.1000 g	0.0000 g	0.15 mg	2
4	0.5000 g	0.5000 g	0.0000 g	0.15 mg	2
5	1.0000 g	1.0000 g	0.0000 g	0.15 mg	2
6	5.0000 g	5.0000 g	0.0000 g	0.16 mg	2
7	10.0000 g	10.0001 g	0.0001 g	0.16 mg	2
8	50.0000 g	50.0000 g	0.0000 g	0.19 mg	2
9	99.9999 g	100.0000 g	0.0001 g	0.25 mg	2
10	149.9999 g	150.0000 g	0.0001 g	0.35 mg	2
11	200.0001 g	200.0003 g	0.0002 g	0.39 mg	2

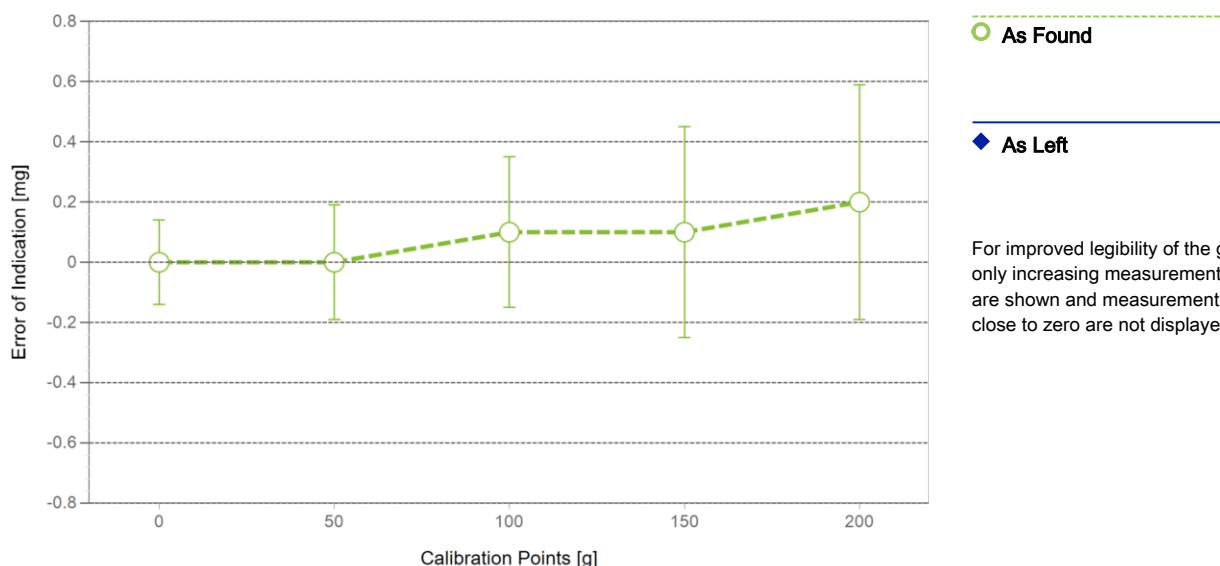

The expanded measurement uncertainty is reported as the standard measurement uncertainty multiplied by the coverage factor k such that the coverage probability corresponds to approximately 95 %.

The user is responsible for maintaining environmental conditions and the settings of the weighing instrument when it was calibrated.
The results of this calibration certificate relate only to the calibrated item.

Test Equipment

All weights used for metrological testing are traceable to national or international standards. The weights were calibrated and certified by an accredited calibration laboratory.

Weight Set 1: OIML E2

Weight Set No.:	WS38	Date of Issue:	15-Dec-2023
Certificate Number:	189517	Calibration Due Date:	15-Jun-2025

Weight Set 2: OIML E2

Weight Set No.:	WS38-1	Date of Issue:	22-Feb-2024
Certificate Number:	C411772496	Calibration Due Date:	22-Aug-2025

Weight Set 3: OIML E2

Weight Set No.:	WS38-3	Date of Issue:	27-Feb-2024
Certificate Number:	C411772498	Calibration Due Date:	27-Aug-2025

Thermo Hygrometer

Equipment No.:	IN256	Date of Issue:	19-Jul-2024
Certificate Number:	SG-H-00636/67	Calibration Due Date:	18-Jul-2025

Remarks

FACT adjustment functionality activated
Equipment condition: Good
Next calibration according to customer's procedure
Calibration data not decide by calibration laboratory

End of Accredited Section

The information below and any attachments to this calibration certificate are not part of the accredited calibration.

Measurement Uncertainty of the Weighing Instrument in Use

Stated is the expanded uncertainty with $k=2$ in use. The formula shall be used for the estimation of the uncertainty under consideration of the errors of indication. The value R represents the net load indication in the unit of measure of the device.

Temperature coefficient for the evaluation of the measurement uncertainty in use: $1.5 \cdot 10^{-6} / K$

Temperature range on site for the evaluation of the measurement uncertainty in use: 3 K


Linearization of Uncertainty Equation

Range			As Found	As Left
	d	Max		
1	0.0001 g	220 g	$U_1 = 0.15 \text{ mg} + 0.00482 \text{ mg/g} \cdot R$	N/A


To optimize the stability of the linearization, besides of the zero load only increasing measurement points with a test load of 5% of the measurement range or larger are taken for the calculation of the linear equation.

Absolute and Relative Measurement Uncertainty in Use for Various Net Indications (Examples)

Net Indication	As Found		As Left	
0.0220 g	0.15 mg	0.68%	N/A	N/A
0.2200 g	0.15 mg	0.069%	N/A	N/A
2.2000 g	0.16 mg	0.0073%	N/A	N/A
22.0000 g	0.26 mg	0.0012%	N/A	N/A
220.0000 g	1.2 mg	0.00055%	N/A	N/A

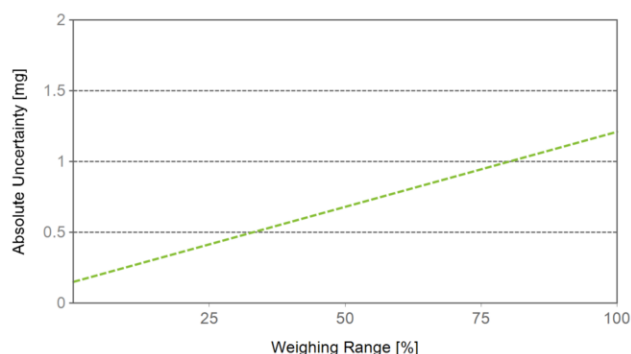

As Found

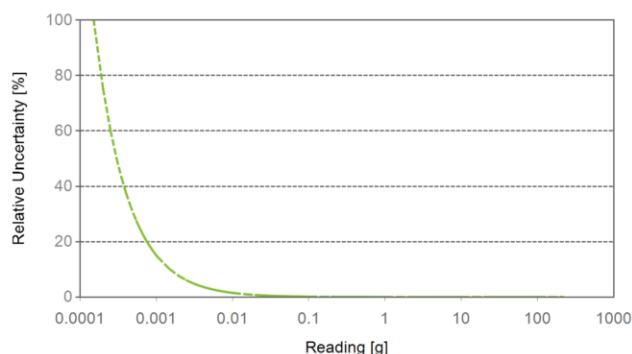

As Left

GWP® Certificate



As
Found



As
Left



The weighing device meets the given process requirements.

The weighing device meets the given process requirements.

Tests Performed:



As Found



As Left



No adjustments/modifications made. As Left results correspond to As Found.


Process Requirements

Weighing Tolerance: 1%

Smallest Net Weight: 0.0500 g

Safety Factor: 2

Safe Weighing Range

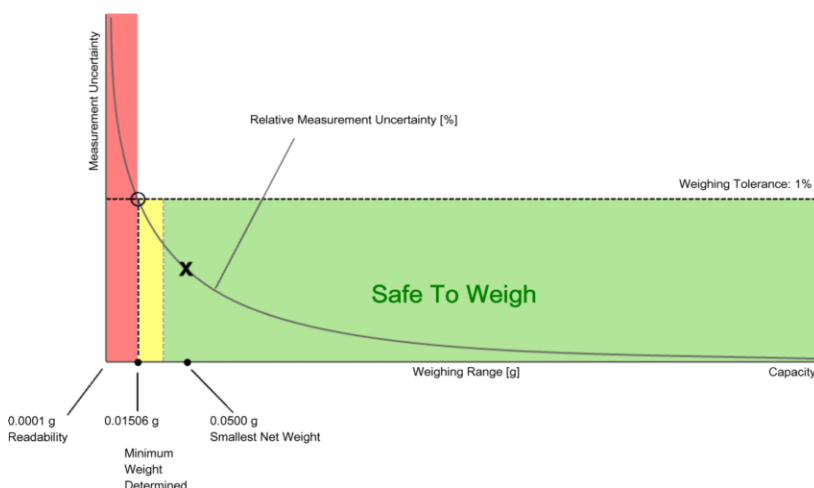

While the values in this graph reflect the actual calibration results, the measurement uncertainty curves are simply a visual representation. This graph reflects As Left testing, unless only As Found was performed.

Minimum Weight

As Found Minimum Weight Table

Minimum weights for different weighing tolerances and safety factors					
	Safety Factor				
Tolerance	1	2	3	5	10
0.1%	0.15128 g	0.30404 g	0.45829 g	0.77136 g	1.58179 g
0.2%	0.07546 g	0.15128 g	0.22748 g	0.38098 g	0.77136 g
0.5%	0.03014 g	0.06034 g	0.09059 g	0.15128 g	0.30404 g
1%	0.01506 g	0.03014 g	0.04523 g	0.07546 g	0.15128 g
2%	0.00753 g	0.01506 g	0.02260 g	0.03768 g	0.07546 g
5%	0.00301 g	0.00602 g	0.00904 g	0.01506 g	0.03014 g



Pass: The determined minimum weight meets the requirement for the smallest net weight.

As Left Minimum Weight Table

Minimum weights for different weighing tolerances and safety factors					
	Safety Factor				
Tolerance	1	2	3	5	10
0.1%	0.15128 g	0.30404 g	0.45829 g	0.77136 g	1.58179 g
0.2%	0.07546 g	0.15128 g	0.22748 g	0.38098 g	0.77136 g
0.5%	0.03014 g	0.06034 g	0.09059 g	0.15128 g	0.30404 g
1%	0.01506 g	0.03014 g	0.04523 g	0.07546 g	0.15128 g
2%	0.00753 g	0.01506 g	0.02260 g	0.03768 g	0.07546 g
5%	0.00301 g	0.00602 g	0.00904 g	0.01506 g	0.03014 g



Pass: The determined minimum weight meets the requirement for the smallest net weight.

At these net minimum weight values, the measurement uncertainty of the weighing device is equal to or less than 1/1 (no safety factor), 1/2, 1/3, 1/5, or 1/10 of the required tolerance. The values are calculated with $k = 2$ and based on the linear formula of the measurement uncertainty of the weighing device in use.

The safety factor for As Found is always 1. This implies no safety factor. As Found testing looks at the behavior of the instrument from the past until test occurred. For the past, it is necessary to know that the tolerance was met, but not the safety factor. The safety factor is a proactive measure to apply for future measurements.

Notes on minimum weight values in above table:

1. If "N/A" is shown above, no appropriate value could be calculated.
2. METTLER TOLEDO is not responsible for the definition of the process requirements.

Measurement Results

Results Summary

	Repeatability	Eccentricity	Error of Indication
As Found	✓	✓	✓
As Left	✓	✓	✓

✓ = Passed

✗ = Failed

⚠ = Safety Factor not met

Repeatability

Test Load: 100 g

Tolerance	Control Limit	As Found		As Left	
		Std. Deviation	Result	Std. Deviation	Result
0.1%	N/A	0.00006 g*	N/A	0.00006 g*	N/A
0.2%	0.00005 g		✗		✗
0.5%	0.00013 g		✓		✓
1%	0.00025 g		✓		✓
2%	0.00050 g		✓		✓
5%	0.00125 g		✓		✓

*The calculated standard deviation value is below the rounding error of the balance. The $0.41 \cdot d$ rule is used for the assessment of this repeatability test and the calculation of the minimum weight.

The weighing tolerance is met if the standard deviation is less than or equal to the corresponding control limit.

Eccentricity

Test Load: 100 g

Tolerance	Control Limit	As Found		As Left	
		Deviation	Result	Deviation	Result
0.1%	0.0500 g	0.0001 g	✓	0.0001 g	✓
0.2%	0.1000 g		✓		✓
0.5%	0.2500 g		✓		✓
1%	0.5000 g		✓		✓
2%	1.0000 g		✓		✓
5%	2.5000 g		✓		✓

The weighing tolerance is met if the deviation is less than or equal to the corresponding control limit.

Error of Indication**As Found**

		Control limits for various weighing tolerances					
Reference Value	Error	0.1%	0.2%	0.5%	1%	2%	5%
0.0000 g	0.0000 g	N/A	N/A	N/A	N/A	N/A	N/A
50.0000 g	0.0000 g	0.0250 g	0.0500 g	0.1250 g	0.2500 g	0.5000 g	1.2500 g
99.9999 g	0.0001 g	0.0500 g	0.1000 g	0.2500 g	0.5000 g	1.0000 g	2.5000 g
149.9999 g	0.0001 g	0.0750 g	0.1500 g	0.3750 g	0.7500 g	1.5000 g	3.7500 g
200.0001 g	0.0002 g	0.1000 g	0.2000 g	0.5000 g	1.0000 g	2.0000 g	5.0000 g
Result		✓	✓	✓	✓	✓	✓

As Left

		Control limits for various weighing tolerances					
Reference Value	Error	0.1%	0.2%	0.5%	1%	2%	5%
0.0000 g	0.0000 g	N/A	N/A	N/A	N/A	N/A	N/A
50.0000 g	0.0000 g	0.0250 g	0.0500 g	0.1250 g	0.2500 g	0.5000 g	1.2500 g
99.9999 g	0.0001 g	0.0500 g	0.1000 g	0.2500 g	0.5000 g	1.0000 g	2.5000 g
149.9999 g	0.0001 g	0.0750 g	0.1500 g	0.3750 g	0.7500 g	1.5000 g	3.7500 g
200.0001 g	0.0002 g	0.1000 g	0.2000 g	0.5000 g	1.0000 g	2.0000 g	5.0000 g
Result		✓	✓	✓	✓	✓	✓

The weighing tolerance is met if the error (of indication) for each test point is less than or equal to the corresponding control limit for that particular weighing tolerance. Results at or close to the zero point cannot be assessed.



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL.0-2717-3000-29 FAX.0-2719-9484



Certificate of Calibration

Cert. No.: 25TM32

Page : 1 of 3

Equipment : Hot Air Oven

Manufacturer : Binder

Model : FED 115 E2

Serial No. : 11-22823

ID No. : ERTC-L-In-076

Submitted by : Environment Research & Technology Company Limited.
25/114 Moo 6, Soi Chinaket 1, Ngamwongwan Road,
Toongsonghong, Laksi,
Bangkok 10210

Location : หน้าห้อง 510

Received Order : 06 January 2025

Calibration Date : 06 January 2025

Ambient Temperature : (26 ± 10) °C

Relative Humidity : (50 ± 30) %

AC Line Voltage : (220 ± 22) V

Calibrated by :

Approved by :

- () Ponpan Paipim
() Suwit Imjai
(✓) Kunchit Promprat

Issue Date :

18 January 2025

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.



Equipment : Hot Air Oven
Condition As-Received : Used Item
Reference : 2501-0004ON-2

Cert. No.: 25TM32

Page : 2 of 3

Procedure Used :-

Calibration were conducted using calibration procedure CP-OT02 based on TLAS G-20 according to direct measurement method with Data Acquisition which connected with Resistance Temperature Detector (RTD) and Thermocouple Type T.

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

<u>Instrument</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Traceable</u>	<u>Due Date</u>
1) Data Acquisition	MY49001451	24LM44	TPA	17 Mar 2025
2) Data Acquisition	MY49001451	24LM79	TPA	29 May 2025

2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certification is traceable to the International System of Unit.


Remark : TPA : Technology Promotion Association (Thailand - Japan)

Result of Calibration :- (*) Without Adjustment

Function of UUC* : Temperature Source

Fresh air setting : Close

Environment during calibration		
	Beginning	Finished
Temp. (°C)	28	27
REL.Humid. (%)	55	58
AC Supply (Volt)	222	221

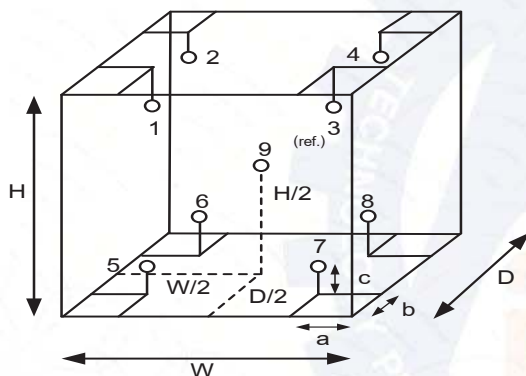

Ref. Std. ID No.: @ Calibration Point		
Position :	(104) °C	(180) °C
1	19RTD-2/1	24-19TC-01
2	19RTD-2/2	24-19TC-02
3	19RTD-2/3	24-19TC-03
4	19RTD-2/4	24-19TC-04
5	19RTD-2/5	24-19TC-05
6	24-19RTD-2/6	24-19TC-06
7	19RTD-2/7	24-19TC-07
8	19RTD-2/8	24-19TC-08
9 (ref.)	19RTD-2/9	24-19TC-09

Probe Installation Details :

a = 5.0 cm
 b = 5.0 cm
 c = 5.0 cm

Dimension of Chamber :

D = 0.40 m
 W = 0.60 m
 H = 0.48 m
 Capacity = 0.12 m³



Equipment : Hot Air Oven
Condition As-Received : Used Item
Reference : 2501-0004ON-2
Result of Calibration :- (*) Without Adjustment
Function of UUC* : Temperature Source
Fresh air setting : Close

Cert. No.: 25TM32

Page : 3 of 3

Calibration Point (°C)	UUC* Setting (°C)	UUC* Reading (°C)	Temperature stability (± °C)	Temperature uniformity (°C)	Overall Variation (°C)	Coverage Factor <i>k</i>
104	104	104	0.13	2.0	2.2	2
180	180	180	0.74	3.8	4.8	2

Calibration Point (°C)	Measured Temperature (°C)									Uncertainty (±°C)
	Position									
	1	2	3	4	5	6	7	8	9 (ref.)	
104	104.727	103.435	104.430	103.878	103.258	102.923	104.882	103.647	102.939	0.80
180	178.529	178.085	181.353	181.341	179.519	177.627	181.808	179.627	178.498	1.7

Average* : The average of 30 values in each position.

Temperature stability : One-half of the greatest maximum difference of measured temperature at any one sensor.

Temperature uniformity : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.

Overall Variation : The Difference of the maximum and minimum measured temperatures throughout observation.

UUC* : Unit Under Calibration

Note : The reported uncertainty of measurement was included stability and excluded uniformity .

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL.0-2717-3000-29 FAX.0-2719-9484



Certificate of Calibration

Cert. No.: 25TM33

Page : 1 of 3

Equipment : Hot Air Oven

Manufacturer : Memmert

Model : UF 110

Serial No. : B414.0652

ID No. : ERTC-L-In-098

Submitted by : Environment Research & Technology Company Limited.
25/114 Moo 6, Soi Chinaket 1, Ngamwongwan Road,
Toongsonghong, Laksi,
Bangkok 10210

Location : หน้าห้อง 510

Received Order : 06 January 2025

Calibration Date : 06 January 2025



Ambient Temperature : (26 ± 10) °C

Relative Humidity : (50 ± 30) %

AC Line Voltage : (220 ± 22) V

Calibrated by :

Approved by :

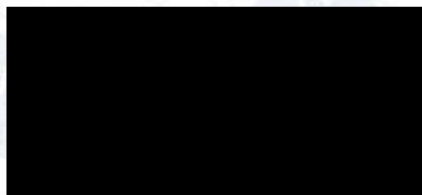

Issue Date :

18 January 2025

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.



Equipment : Hot Air Oven
Condition As-Received : Used Item
Reference : 2501-0004ON-3

Cert. No.: 25TM33

Page : 2 of 3

Procedure Used :-

Calibration were conducted using calibration procedure CP-OT02 based on TLAS G-20 according to direct measurement method with Data Acquisition which connected with Resistance Temperature Detector (RTD) and Thermocouple Type T.

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

<u>Instrument</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Traceable</u>	<u>Due Date</u>
1) Data Acquisition	MY49001451	24LM44	TPA	17 Mar 2025
2) Data Acquisition	MY49001451	24LM79	TPA	29 May 2025

2. This certificate is valid only to the item calibrated on date and place of calibration.


3. This certification is traceable to the International System of Unit.

Remark : TPA : Technology Promotion Association (Thailand - Japan)

Result of Calibration :- (*) Without Adjustment

Function of UUC* : Temperature Source

Fresh air setting : Close

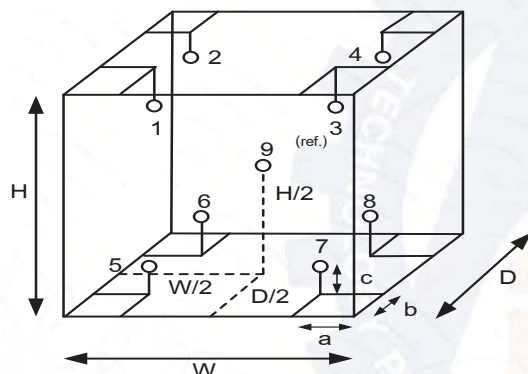

Environment during calibration		
	Beginning	Finished
Temp. (°C)	28	27
REL.Humid. (%)	55	58
AC Supply (Volt)	222	221

Ref. Std. ID No.: @ Calibration Point		
Position :	(104) °C	(180) °C
1	19RTD-2/1	24-19TC-01
2	19RTD-2/2	24-19TC-02
3	19RTD-2/3	24-19TC-03
4	19RTD-2/4	24-19TC-04
5	19RTD-2/5	24-19TC-05
6	24-19RTD-2/6	24-19TC-06
7	19RTD-2/7	24-19TC-07
8	19RTD-2/8	24-19TC-08
9 (ref.)	19RTD-2/9	24-19TC-09

Probe Installation Details :

a = 5.0 cm
b = 5.0 cm
c = 5.0 cm

Dimension of Chamber :

D = 0.40 m
W = 0.56 m
H = 0.48 m
Capacity = 0.11 m³



Equipment : Hot Air Oven
Condition As-Received : Used Item
Reference : 2501-0004ON-3
Result of Calibration :- (*) Without Adjustment
Function of UUC* : Temperature Source
Fresh air setting : Close

Cert. No.: 25TM33

Page : 3 of 3

Calibration Point (°C)	UUC* Setting (°C)	UUC* Reading (°C)	Temperature stability (± °C)	Temperature uniformity (°C)	Overall Variation (°C)	Coverage Factor <i>k</i>
104.0	104.0	104.0	0.13	1.2	1.8	2
180.0	180.0	180.0	0.54	3.6	4.7	2

Calibration Point (°C)	Measured Temperature (°C)									Uncertainty (±°C)
	Position									
	1	2	3	4	5	6	7	8	9 (ref.)	
104.0	104.884	103.140	103.191	103.508	104.382	103.829	104.340	103.742	104.282	0.42
180.0	181.068	177.733	178.025	179.100	181.089	180.099	181.795	180.145	181.130	1.4

Average* : The average of 30 values in each position.

Temperature stability : One-half of the greatest maximum difference of measured temperature at any one sensor.

Temperature uniformity : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.

Overall Variation : The Difference of the maximum and minimum measured temperatures throughout observation.

UUC* : Unit Under Calibration

Note : The reported uncertainty of measurement was included stability and excluded uniformity .

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

Preventive Maintenance Block Digestion

Service No. PM25-S08-151

1. Customer Information

Customer Name	Instrument	Serial Number	Service Date
บริษัท เอ็นไวรอนเมนต์ รีเสิร์ช แอนด์ เทคโนโลยี จำกัด 25/114 หมู่ที่ 6 ซอยชินเขต 1, งามวงศ์วาน แขวงทุ่งสองห้อง เขตหลักสี่ กรุงเทพมหานคร 10210 ติดต่อ คุณยุวดี Tel: 095-632-9445 Fax:	K-449	1000299283	06 Jun 2025 PM 1/2

2. Instrument

	OK	NOT OK	Remark
2.1 Housing			
- Clean the housing	/		
- Visual check	/		
- Check for defects (e.g. cracks)	/		

	OK	NOT OK	Remark
2.2 Heating			
- Clean aluminum block	/		
- Visual check	/		
- Check heating element	/		

Preventive Maintenance Block Digestion

2.3 Visual Check	OK	NOT OK	Remark
- Connection to suction	/		
- PTFE seal	/		
- O-ring	/		
- Glass holder set	/		
- Suction module	/		

2.4 Function test (This test does not use digestion vessels!)



- Select and store in .Program 9 by following parameters:
 - o Step 1 Ramp 1 Temp. 55°C Time 2 min.
 - o Step 2 Ramp 2 Temp. 70°C Time 2 min.
 - o Step 3 Ramp 3 Temp. 85°C Time 2 min.
 - o Step 4 Ramp 4 Temp. 100°C Time 2 min.
 - o Step 5 Cool Time 10 min.
- Check following functions:
 - o Press key "Start": Start Time 00.00
 - o 0 min. press key .Start. again starts heating from room temperature (LED Heating on)
 - o 5 min. reaches 55°C (LED off) Lift goes down (K-438 only)
 - o 6 min. starts heating again (LED on)
 - o 7 min. reaches 70°C (LED off)
 - o 8 min. starts heating again (LED on)
 - o 9 min. reaches 85°C (LED off)
 - o 10 min. starts heating again (LED on)
 - o 11 min. reaches 100°C (LED off)
 - o 12 min. starts cooling (fan on) Lift goes up (K-438 only)
 - o 22 min. End / Scrubber off; LED still flashing displays 'power off delay - cooling' (Instrument will switch off automatically, if temperature of the heating block drops below 60°C)
- Note:
 - o This are only approximate times starting from room temperature and they can vary slightly!
 - o Not all heating positions have exactly the same heating output! (Constructive matter)
 - o Temperatures may overshoot set temperatures. (only below 100°C)

Function test

☒ OK

☐ NOT OK



BUCHI (Thailand) Limited

Preventive Maintenance Block Digestion

2.5 System control	OK	NOT OK	Remark
- Keyboard	/		
- Display	/		
- Program	/		

3. Summary

All specifications OK	Specification not OK
OK	



Comments

PM 1/2

เครื่องใช้งานได้ปกติ งานเป็นปกติ งานเป็นปกติ

Signature BUCHI

- Service by _____

Date 06 Jun 2025

- Approve by _____

Date 06 Jun 2025



BUCHI (Thailand) Limited

Preventive Maintenance Kjeldahl

Service No. PM25-S08-151

1. Customer Information

Customer Name	Instrument	Serial Number	Service Date
บริษัท เอ็นไวรอนเม้นท์ รีเสิร์ช แอนด์ เทคโนโลยี จำกัด 25/114 หมู่ที่ 6 ซอยชินเขต 1, งามวงศ์วาน แขวงทุ่งสองห้อง เขตหลักสี่ กรุงเทพมหานคร 10210 ติดต่อ คุณยุวดี Tel: 095-632-9445 Fax:	K-355	1000142231	06 Jun 2025 PM 1/2

2. Instrument

2.1 Cooling water (If it connected)	OK	NOT OK	Remark
- Temperature 15 – 20 °C	/		
- Cooling water inlet	/		
- Cooling water outlet	/		
- Control Temperature	/		

2.2 Cleaning	DONE	NOT DONE	Remark
- Outside Instrument	/		
- Inside Instrument	/		
- Splash protector	/		
- Condenser	/		

Preventive Maintenance Kjeldahl

2.3 Visual Test	OK	NOT OK	Remark
- Screw Coupling (between splash protector and condenser)	/		
- Condenser	/		
- Splash protector	/		
- Hypalon connection (connection tube)	/		
- Rubber bung	/		
- Ventilation valve	/		
- PTFE tube	/		
- Cooling water inlet	/		
- Cooling water outlet	/		
- Magnetic valve	/		

2.4 System control	OK	NOT OK	Remark
- Key board	/		
- Display	/		
- Program	/		
- Adding H ₂ O	/		
- Adding NaOH	/		
- Adding H ₃ BO ₃	/		
- Aspiration	/		

Preventive Maintenance Kjeldahl



2.5 System Distillation	OK	NOT OK	Remark
- Boiler	/		
- Water level sensor	/		
- One way valve	/		
- Pressure switch	/		
- Thermostat	/		
- Steam valve1 (Y4)	/		
- Steam valve2 (Y5)	/		
- Drain valve (Y3)	/		
- Water 3/2 way valve (Y1)	/		

2.6 Hose	OK	NOT OK	Remark
- Unisil hose	/		
- Hypalon hose	/		
- Drain hose	/		
- Viton hose	/		
- Silicone hose	/		

2.7 Diaphragm pump	OK	NOT OK	Remark
- Diaphragm pump for H ₂ O	/		
- Diaphragm pump for NaOH	/		
- Diaphragm pump for H ₃ BO ₃	/		

2.8 Program test	OK	NOT OK	Remark
- Distillation	/		
- Aspiration	/		
- Preheating	/		
- Cleaning	/		

Preventive Maintenance Kjeldahl

3. Function Test

Addition H ₂ O	0 ml	Reaction time	0 min
Addition NaOH	0 ml	Distillation time	5 min
Addition H ₃ BO ₃	0 ml	Steam capacity	100%
		Aspiration	SAM

Result: Water in receiving vessel now approximately 170 ml, 175 ml

4. Summary



All specifications OK	Specification not OK
OK	


Comments

PM 1/2

เครื่องใช้งานได้ปกติ


Signature BUCHI

- Service by



Date 06 Jun 2025

- Approve by



Date 06 Jun 2025



Mettler-Toledo (Thailand) Ltd.

846/4 - 846/5 Lasalle Rd., Bangna Tai Sub-District

Bangna District, Bangkok 10260

+662 723 0382

MT-TH.ServiceSupport@mt.com



NSC-TISI-TIS 17025
CALIBRATION 0062

Accuracy Calibration Certificate

Customer

Company: Environment Research & Technology
Address: 25/114 Moo 6, Soi Chinaket 1, Ngamwongwan Rd., Toongsonghong
City: Laksi **Contact:** Ramita Taengthai
Zip / Postal: 10210
State / Province: Bangkok
Order Number: 
0 3 3 3 6 1 0 1 9

Weighing Device

Manufacturer: Mettler Toledo **Instrument Type:** Weighing Instrument
Model: MS204TS/00 **Asset Number:** ERTC-L-IN-114
Serial No.: B547728937 **Terminal Model:** N/A
Building: N/A **Terminal Serial No.:** N/A
Floor: 5 **Terminal Asset No.:** N/A
Room: 504

Range	Max. Capacity	Readability (d)
1	220 g	0.0001 g

Procedure

Calibration Guideline: EURAMET cg-18 v. 4.0/CENAM-ema:2015
METTLER TOLEDO Work Instruction: CP/W002/20


This calibration certificate contains measurements for As Found calibration. No As Left calibration was performed because the device was not modified after As Found calibration. Therefore, results for As Left correspond to As Found.

The sensitivity/span of the weighing instrument was adjusted before calibration with a built-in weight.

In accordance with EURAMET cg-18 (11/2015), the test loads were selected to reflect the specific use of the weighing device or to accommodate specific calibration conditions.

	Temperature		Humidity	
As Found	Start: 21.1 °C	End: 20.3 °C	Start: 37.8 %	End: 42.2 %

As Found Calibration Date: 15-Jan-2025
As Left Calibration Date: N/A
Issue Date: 17-Jan-2025

Calibrator: 
Approved Signatory: 
Technical Manager / Head of Calibration Center

Measurement Results


Repeatability

Test Load: 100 g

	As Found	As Left
1	99.9999 g	N/A
2	99.9999 g	N/A
3	99.9999 g	N/A
4	99.9998 g	N/A
5	100.0000 g	N/A
6	99.9999 g	N/A
7	99.9999 g	N/A
8	99.9999 g	N/A
9	99.9998 g	N/A
10	99.9999 g	N/A

Standard Deviation	0.00006 g	N/A
--------------------	-----------	-----

○ As Found
◆ As Left

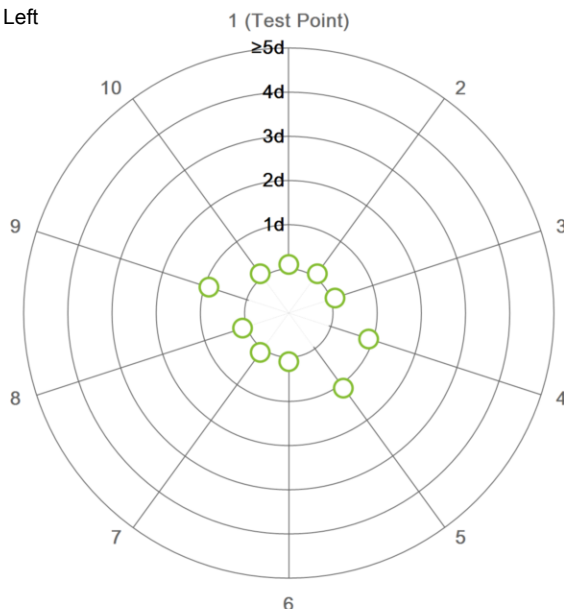

The "d" in the graph represents the readability of the range/interval in which the test was performed.


The results of this graph are based upon the absolute values of the differences from the mean value.

Eccentricity

Test Load: 100 g

Position	As Found	As Left
1	99.9999 g	N/A
2	99.9999 g	N/A
3	100.0000 g	N/A
4	99.9998 g	N/A
5	99.9999 g	N/A

Maximum Deviation	0.0001 g	N/A
-------------------	----------	-----




As Found

The "d" in the graph represents the readability of the range/interval in which the test was performed.

Error of Indication

As Found

	Reference Value	Indication	Error of Indication	Expanded Uncertainty	k
1	0.0000 g	0.0000 g	0.0000 g	0.13 mg	2
2	0.0500 g	0.0500 g	0.0000 g	0.14 mg	2
3	0.1000 g	0.1000 g	0.0000 g	0.14 mg	2
4	0.5000 g	0.5000 g	0.0000 g	0.14 mg	2
5	1.0000 g	1.0000 g	0.0000 g	0.14 mg	2
6	5.0000 g	5.0000 g	0.0000 g	0.15 mg	2
7	10.0000 g	10.0000 g	0.0000 g	0.15 mg	2
8	50.0000 g	50.0000 g	0.0000 g	0.18 mg	2
9	99.9999 g	100.0000 g	0.0001 g	0.24 mg	2
10	149.9999 g	150.0000 g	0.0001 g	0.35 mg	2
11	200.0001 g	200.0002 g	0.0001 g	0.39 mg	2

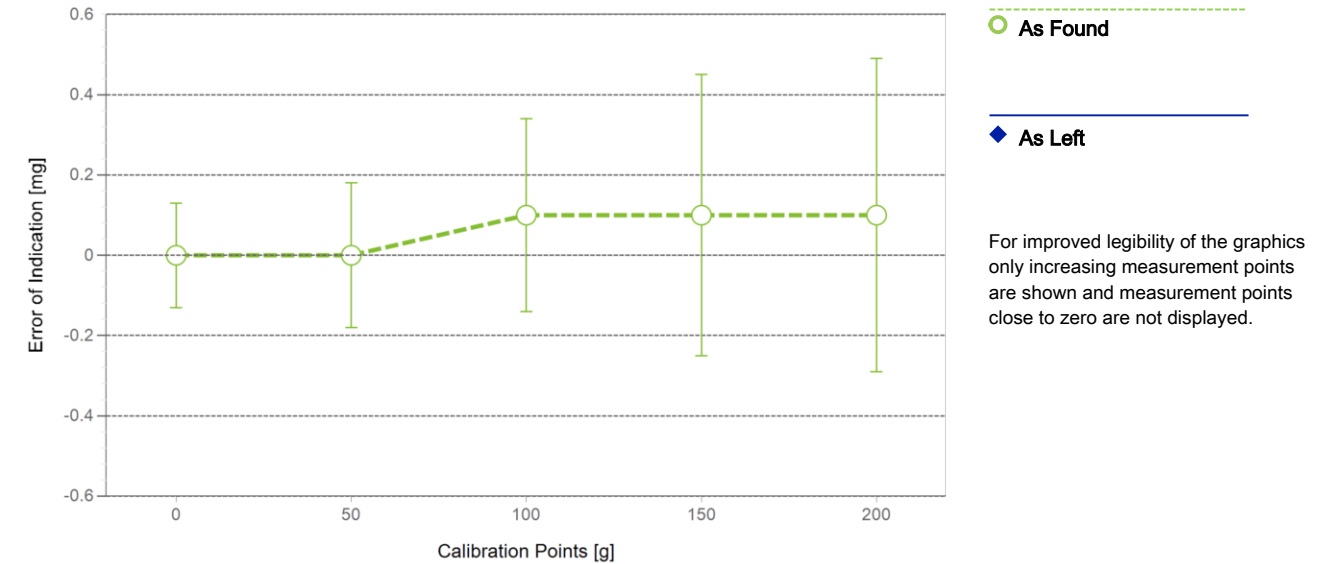

The expanded measurement uncertainty is reported as the standard measurement uncertainty multiplied by the coverage factor k such that the coverage probability corresponds to approximately 95 %.

The user is responsible for maintaining environmental conditions and the settings of the weighing instrument when it was calibrated.

The results of this calibration certificate relate only to the calibrated item.

Test Equipment

All weights used for metrological testing are traceable to national or international standards. The weights were calibrated and certified by an accredited calibration laboratory.

Weight Set 1: OIML E2

Weight Set No.:	WS38	Date of Issue:	15-Dec-2023
Certificate Number:	189517	Calibration Due Date:	15-Jun-2025

Weight Set 2: OIML E2

Weight Set No.:	WS38-1	Date of Issue:	22-Feb-2024
Certificate Number:	C411772496	Calibration Due Date:	22-Aug-2025

Weight Set 4: OIML E2

Weight Set No.:	WS38-3	Date of Issue:	27-Feb-2024
Certificate Number:	C411772498	Calibration Due Date:	27-Aug-2025

Thermo Hygrometer

Equipment No.:	IN256	Date of Issue:	19-Jul-2024
Certificate Number:	SG-H-00636/67	Calibration Due Date:	18-Jul-2025

Remarks

FACT adjustment functionality activated
Equipment condition: Good
Next calibration according to customer's procedure
Calibration data not decide by calibration laboratory

End of Accredited Section

The information below and any attachments to this calibration certificate are not part of the accredited calibration.

Measurement Uncertainty of the Weighing Instrument in Use

Stated is the expanded uncertainty with k=2 in use. The formula shall be used for the estimation of the uncertainty under consideration of the errors of indication. The value R represents the net load indication in the unit of measure of the device.

Temperature coefficient for the evaluation of the measurement uncertainty in use: 3.0 · 10⁻⁶ / K

Temperature range on site for the evaluation of the measurement uncertainty in use: 3 K


Linearization of Uncertainty Equation

Range			As Found	As Left
	d	Max		
1	0.0001 g	220 g	$U_1 = 0.14 \text{ mg} + 0.00647 \text{ mg/g} \cdot R$	N/A


To optimize the stability of the linearization, besides of the zero load only increasing measurement points with a test load of 5% of the measurement range or larger are taken for the calculation of the linear equation.

Absolute and Relative Measurement Uncertainty in Use for Various Net Indications (Examples)

Net Indication	As Found		As Left	
0.0220 g	0.14 mg	0.64%	N/A	N/A
0.2200 g	0.14 mg	0.064%	N/A	N/A
2.2000 g	0.15 mg	0.0070%	N/A	N/A
22.0000 g	0.28 mg	0.0013%	N/A	N/A
220.0000 g	1.6 mg	0.00071%	N/A	N/A

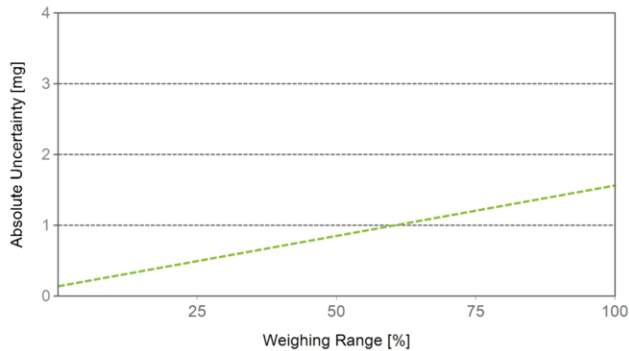

As Found

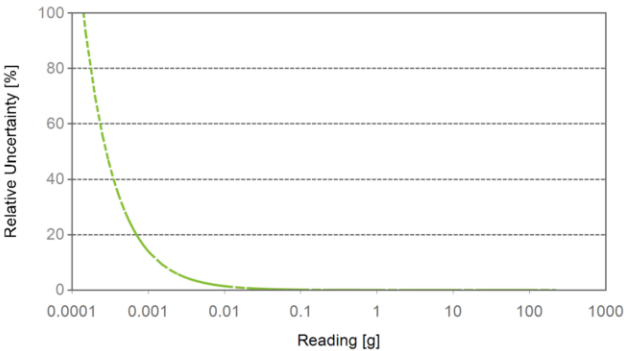

As Left

GWP® Certificate



As
Found



As
Left



The weighing device meets the given process requirements.

The weighing device meets the given process requirements.

Tests Performed:



As Found



As Left



No adjustments/modifications made. As Left results correspond to As Found.


Process Requirements

Weighing Tolerance: 1%

Smallest Net Weight: 0.0500 g

Safety Factor: 2

Safe Weighing Range

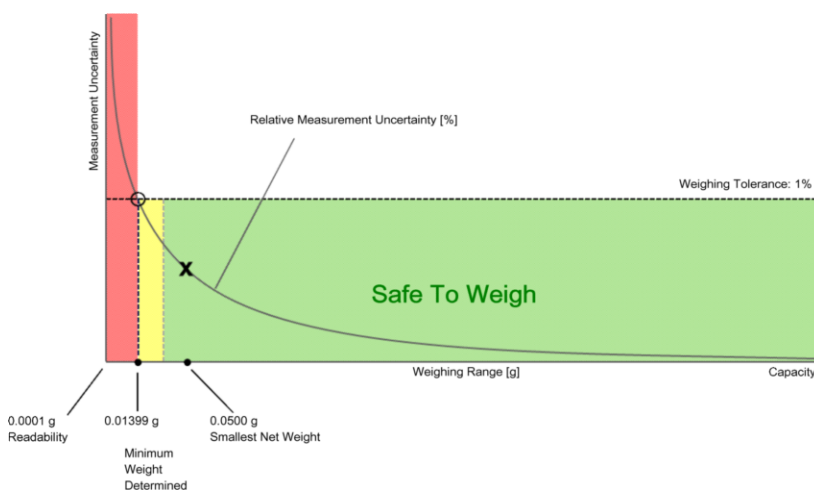

While the values in this graph reflect the actual calibration results, the measurement uncertainty curves are simply a visual representation. This graph reflects As Left testing, unless only As Found was performed.

Minimum Weight

As Found Minimum Weight Table

Minimum weights for different weighing tolerances and safety factors					
	Safety Factor				
Tolerance	1	2	3	5	10
0.1%	0.14075 g	0.28335 g	0.42783 g	0.72259 g	1.49521 g
0.2%	0.07015 g	0.14075 g	0.21182 g	0.35535 g	0.72259 g
0.5%	0.02800 g	0.05608 g	0.08423 g	0.14075 g	0.28335 g
1%	0.01399 g	0.02800 g	0.04203 g	0.07015 g	0.14075 g
2%	0.00699 g	0.01399 g	0.02100 g	0.03502 g	0.07015 g
5%	0.00280 g	0.00560 g	0.00839 g	0.01399 g	0.02800 g



Pass: The determined minimum weight meets the requirement for the smallest net weight.

As Left Minimum Weight Table

Minimum weights for different weighing tolerances and safety factors					
	Safety Factor				
Tolerance	1	2	3	5	10
0.1%	0.14075 g	0.28335 g	0.42783 g	0.72259 g	1.49521 g
0.2%	0.07015 g	0.14075 g	0.21182 g	0.35535 g	0.72259 g
0.5%	0.02800 g	0.05608 g	0.08423 g	0.14075 g	0.28335 g
1%	0.01399 g	0.02800 g	0.04203 g	0.07015 g	0.14075 g
2%	0.00699 g	0.01399 g	0.02100 g	0.03502 g	0.07015 g
5%	0.00280 g	0.00560 g	0.00839 g	0.01399 g	0.02800 g



Pass: The determined minimum weight meets the requirement for the smallest net weight.

At these net minimum weight values, the measurement uncertainty of the weighing device is equal to or less than 1/1 (no safety factor), 1/2, 1/3, 1/5, or 1/10 of the required tolerance. The values are calculated with $k = 2$ and based on the linear formula of the measurement uncertainty of the weighing device in use.

The safety factor for As Found is always 1. This implies no safety factor. As Found testing looks at the behavior of the instrument from the past until test occurred. For the past, it is necessary to know that the tolerance was met, but not the safety factor. The safety factor is a proactive measure to apply for future measurements.

Notes on minimum weight values in above table:

1. If "N/A" is shown above, no appropriate value could be calculated.
2. METTLER TOLEDO is not responsible for the definition of the process requirements.

Measurement Results

Results Summary

	Repeatability	Eccentricity	Error of Indication
As Found	✓	✓	✓
As Left	✓	✓	✓

✓ = Passed

✗ = Failed

⚠ = Safety Factor not met

Repeatability

Test Load: 100 g

Tolerance	Control Limit	As Found		As Left	
		Std. Deviation	Result	Std. Deviation	Result
0.1%	N/A	0.00006 g*	N/A	0.00006 g*	N/A
0.2%	0.00005 g		✗		✗
0.5%	0.00013 g		✓		✓
1%	0.00025 g		✓		✓
2%	0.00050 g		✓		✓
5%	0.00125 g		✓		✓

*The calculated standard deviation value is below the rounding error of the balance. The $0.41 \cdot d$ rule is used for the assessment of this repeatability test and the calculation of the minimum weight.

The weighing tolerance is met if the standard deviation is less than or equal to the corresponding control limit.

Eccentricity

Test Load: 100 g

Tolerance	Control Limit	As Found		As Left	
		Deviation	Result	Deviation	Result
0.1%	0.0500 g	0.0001 g	✓	0.0001 g	✓
0.2%	0.1000 g		✓		✓
0.5%	0.2500 g		✓		✓
1%	0.5000 g		✓		✓
2%	1.0000 g		✓		✓
5%	2.5000 g		✓		✓

The weighing tolerance is met if the deviation is less than or equal to the corresponding control limit.

Error of Indication**As Found**

		Control limits for various weighing tolerances					
Reference Value	Error	0.1%	0.2%	0.5%	1%	2%	5%
0.0000 g	0.0000 g	N/A	N/A	N/A	N/A	N/A	N/A
50.0000 g	0.0000 g	0.0250 g	0.0500 g	0.1250 g	0.2500 g	0.5000 g	1.2500 g
99.9999 g	0.0001 g	0.0500 g	0.1000 g	0.2500 g	0.5000 g	1.0000 g	2.5000 g
149.9999 g	0.0001 g	0.0750 g	0.1500 g	0.3750 g	0.7500 g	1.5000 g	3.7500 g
200.0001 g	0.0001 g	0.1000 g	0.2000 g	0.5000 g	1.0000 g	2.0000 g	5.0000 g
Result		✓	✓	✓	✓	✓	✓

As Left

		Control limits for various weighing tolerances					
Reference Value	Error	0.1%	0.2%	0.5%	1%	2%	5%
0.0000 g	0.0000 g	N/A	N/A	N/A	N/A	N/A	N/A
50.0000 g	0.0000 g	0.0250 g	0.0500 g	0.1250 g	0.2500 g	0.5000 g	1.2500 g
99.9999 g	0.0001 g	0.0500 g	0.1000 g	0.2500 g	0.5000 g	1.0000 g	2.5000 g
149.9999 g	0.0001 g	0.0750 g	0.1500 g	0.3750 g	0.7500 g	1.5000 g	3.7500 g
200.0001 g	0.0001 g	0.1000 g	0.2000 g	0.5000 g	1.0000 g	2.0000 g	5.0000 g
Result		✓	✓	✓	✓	✓	✓

The weighing tolerance is met if the error (of indication) for each test point is less than or equal to the corresponding control limit for that particular weighing tolerance. Results at or close to the zero point cannot be assessed.



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL.0-2717-3000-29 FAX.0-2719-9484



Certificate of Calibration

Cert. No.: 25TM35

Page : 1 of 3

Equipment : Incubator

Manufacturer : Memmert

Model : IF 160

Serial No. : D522.0070

ID No. : ERTC-L-In-181

Submitted by : Environment Research & Technology Company Limited
25/114 Moo 6 Soi Chinaket 1,
Ngamwongwan Road, Toongsonghong, Laksi,
Bangkok 10210

Location : 408/2 ห้องปฏิบัติการบ่มอาหารเลี้ยงเชื้อ

Received Order : 06 January 2025

Calibration Date : 06 - 07 January 2025


Ambient Temperature : (26 ± 10) °C

Relative Humidity : (50 ± 30) %

AC Line Voltage : (220 ± 22) V

Calibrated by :

Approved by :

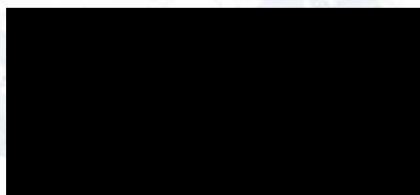

Issue Date :

18 January 2025

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.



Equipment : Incubator
Condition As-Received : Used Item
Reference : 2501-0004ON-5

Cert. No.: 25TM35

Page : 2 of 3

Procedure Used :-

Calibration were conducted using calibration procedure CP-OT02 based on TLAS G-20 according to direct measurement method with Data Acquisition which connected with Resistance Temperature Detector (RTD).

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

Instrument	Serial No.	Cert. No.	Traceable	Due Date
1) Data Acquisition	MY49001451	24LM44	TPA	17 Mar 2025

2. This certificate is valid only to the item calibrated on date and place of calibration.


3. This certification is traceable to the International System of Unit.

Remark : TPA : Technology Promotion Association (Thailand - Japan)

Result of Calibration :- (*) Without Adjustment

Function of UUC* : Temperature Source

Fresh air setting : Close

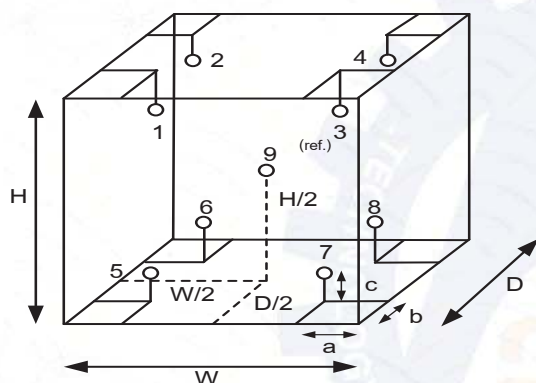

Environment during calibration		
	Beginning	Finished
Temp. (°C)	25	26
REL.Humid. (%)	51	55
AC Supply (Volt)	221	222

Position :	Ref. Std. ID No.:
1	19RTD-2/1
2	19RTD-2/2
3	19RTD-2/3
4	19RTD-2/4
5	19RTD-2/5
6	24-19RTD-2/6
7	19RTD-2/7
8	19RTD-2/8
9 (ref.)	19RTD-2/9

Probe Installation Details :

a = 5.0 cm
b = 5.0 cm
c = 5.0 cm

Dimension of Chamber :

D = 0.40 m
W = 0.56 m
H = 0.73 m
Capacity = 0.16 m³



Equipment : Incubator
Condition As-Received : Used Item
Reference : 2501-0004ON-5
Result of Calibration :- (*) Without Adjustment
Function of UUC* : Temperature Source
Fresh air setting : Close

Cert. No.: 25TM35

Page : 3 of 3

Calibration Point (°C)	UUC* Setting (°C)	UUC* Reading (°C)	Temperature stability (± °C)	Temperature uniformity (°C)	Overall Variation (°C)	Coverage Factor <i>k</i>
35.0	35.0	35.0	0.022	0.22	0.38	2

Calibration Point (°C)	Measured Temperature (°C)									Uncertainty (± °C)
	Position									
	1	2	3	4	5	6	7	8	9 (ref.)	
35.0	34.860	34.762	34.658	34.926	34.791	34.970	34.621	34.837	34.767	0.30

Average* : The average of 30 values in each position.

Temperature stability : One-half of the greatest maximum difference of measured temperature at any one sensor.

Temperature uniformity : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.

Overall Variation : The Difference of the maximum and minimum measured temperatures throughout observation.

UUC* : Unit Under Calibration

Note : The reported uncertainty of measurement was included stability and excluded uniformity .

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL.0-2717-3000-29 FAX.0-2719-9484



Certificate of Calibration

Cert. No.: 25TM36

Page : 1 of 3

Equipment : Incubator

Manufacturer : Ehret

Model : BK 4106

Serial No. : 22162

ID No. : ERTC-L-In-022

Submitted by : Environment Research & Technology Company Limited
25/114 Moo 6 Soi Chinaket 1,
Ngamwongwan Road, Toongsonghong, Laksi,
Bangkok 10210

Location : 408/2 ห้องปฏิบัติการบ่มอาหารเลี้ยงเชื้อ

Received Order : 06 January 2025

Calibration Date : 07 - 08 January 2025

Ambient Temperature : (26 ± 10) °C

Relative Humidity : (50 ± 30) %

AC Line Voltage : (220 ± 22) V

Calibrated by :

Approved by :

Issue Date :

18 January 2025

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.



Equipment : Incubator
Condition As-Received : Used Item
Reference : 2501-0004ON-6

Cert. No.: 25TM36

Page : 2 of 3

Procedure Used :-

Calibration were conducted using calibration procedure CP-OT02 based on TLAS G-20 according to direct measurement method with Data Acquisition which connected with Resistance Temperature Detector (RTD).

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

Instrument	Serial No.	Cert. No.	Traceable	Due Date
1) Data Acquisition	MY49001451	24LM44	TPA	17 Mar 2025

2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certification is traceable to the International System of Unit.


Remark : TPA : Technology Promotion Association (Thailand - Japan)

Result of Calibration :- (*) Without Adjustment

Function of UUC* : Temperature Source

Fresh air setting : Not Available

Environment during calibration		
	Beginning	Finished
Temp. (°C)	26	28
REL.Humid. (%)	53	50
AC Supply (Volt)	222	221

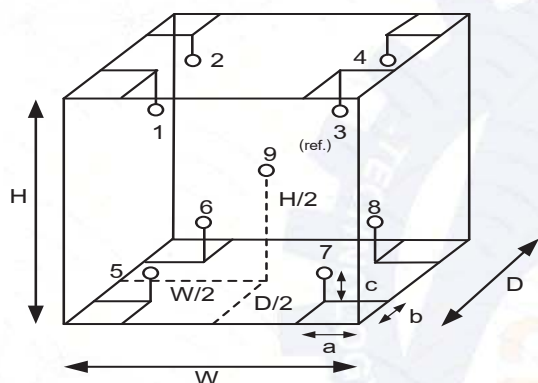

Position :	Ref. Std. ID No.:
1	19RTD-2/1
2	19RTD-2/2
3	19RTD-2/3
4	19RTD-2/4
5	19RTD-2/5
6	24-19RTD-2/6
7	19RTD-2/7
8	19RTD-2/8
9 (ref.)	19RTD-2/9

Probe Installation Details :

a = 5.0 cm
b = 5.0 cm
c = 5.0 cm

Dimension of Chamber :

D = 0.50 m
W = 0.60 m
H = 0.50 m
Capacity = 0.15 m³



Equipment : Incubator
Condition As-Received : Used Item
Reference : 2501-0004ON-6
Result of Calibration :- (*) Without Adjustment
Function of UUC* : Temperature Source
Fresh air setting : Not Available

Cert. No.: 25TM36

Page : 3 of 3

Calibration Point (°C)	UUC* Setting (°C)	UUC* Reading (°C)	Temperature stability (± °C)	Temperature uniformity (°C)	Overall Variation (°C)	Coverage Factor <i>k</i>
44.5	44.5	44.5	0.16	0.64	1.4	2

Calibration Point (°C)	Measured Temperature (°C)									Uncertainty (± °C)
	Position									
	1	2	3	4	5	6	7	8	9 (ref.)	
44.5	44.542	44.705	44.204	44.943	43.855	44.307	44.130	44.630	44.330	0.67

Average* : The average of 30 values in each position.

Temperature stability : One-half of the greatest maximum difference of measured temperature at any one sensor.

Temperature uniformity : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.

Overall Variation : The Difference of the maximum and minimum measured temperatures throughout observation.

UUC* : Unit Under Calibration

Note : The reported uncertainty of measurement was included stability and excluded uniformity .

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-