

ภาคผนวก จ
ใบรับรองการสอบเทียบเครื่องมือ

บริษัท ยูไนเต็ด แอนนาลิสต์ แอนด์ เอ็นจิเนียริง
คอนซัลแตนท์ จำกัด

List of Instruments Certification for Air & Noise Quality Analysis

No.	Instrument/Equipment	Parameter	Manufacturer	Model/Serial No.	Calibrator	Certification No.	Date of Calibration	Due date of Calibration	Remark
Stack									
1	Pre-Test Console	Total Suspended Particulate Hydrogen Sulphide Methyl Mercaptan Dimethyl sulfide	Apex Instruments, USA.	XC-572-V 0803018	Envi Equipment Service Co., Ltd.	E25-010007	16 Jan 25	15 Jan 26	-
2	Flue gas Analyzer	Sulphur Dioxide Oxide of Nitrogen as Nitrogen Dioxide Carbon Monoxide	Testo AG	Testo 350 62289477/0420	Entech Industrial Solution Co., Ltd.	G 680378	12 Jun 25	11 Jun 26	-

List of Opacity Training Certification for Opacity Measurement

No.	Name	Training Course	Train	Date	Remark
1	Mr.Apiwich Toungtee	Opacity	Pollution Control Department	12-13 March 2015	-
2	Mr.Noppasin Thanuthammarat	Opacity	Pollution Control Department	30-31 March 2017	-

List of Instruments Certification for Water Quality Analysis

No.	Instrument/Equipment	Parameter	Manufacturer	Model/Serial No.	Calibrator	Certification No.	Date of Calibration	Due date of Calibration	Remark
Water									
1	pH Meter	pH	Horiba	LAQUA-PH210 HA0F0026	Technology Promotion Association (Thailand-Japan)	25CH22	9 Jan 25	8 Jan 26	-
2	Conductivity Meter	Conductivity	Horiba	LAQUA-EC210 HC0J0015	Technology Promotion Association (Thailand-Japan)	25CH53	15 Jan 25	14 Jan 26	-

Envi Equipment Service Co., Ltd.

110/254 Moo 3, Tumbon Bang Rak Phatthana, Amphur Bang Bua Thong, Nonthaburi 11110

Tel. 098 362 9152, 089 478 7885

E-mail: sales@envi-ees.com

Certificate No.: E25-010007

Page.: 1 of 6

CERTIFICATE OF CALIBRATION

Customer : United Analyst and Engineering Consultant Co., Ltd.
Address : 81 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Description of Equipment : Console meter
Manufacturer : Apex Instrument
Model Number : XC-572-V
Serial Number : 0803018
ID./Control No. : UAE.ANV.193/2551
Environment Conditions : **Temperature** (25 ± 2) °C
: **Humidity** (50 ± 15) % RH
Cal. Date : 16/01/2025
Issue Date : 16/01/2025

Calibration Method or Calibration Procedure Used

US EPA Method (United State Environmental Protection Agency)

This certificate is traceable to national standard, which realize the units of measurement according to the International System of Units (IS).

Result of Calibration

This certificate may not be reproduced other than in full except with prior Written approval of the Technical Manager, Envi Equipment Service Company Limited.

These reported uncertainties of measurement are expanded by a coverage factor of k=2, providing a 95% confidence level

Calibrated by : Mr. Sanya Sangnil

Approved by : _____

(Mr. Mana Fuekha)

Technical Manger

เอกสารไม่ควบคุม



**METHOD 5 CONSOLE CALIBRATION
USING REFERENCE WET GAS METER W-NK-2.5-B-Z No.547425
5-POINT METRIC UNIT**

Meter Console Information	
Console Model Number	XC-572-V
Console Serial Number	0803018
DGM Model Number	SK25EX
DGM Serial Number	00009766

Calibration Conditions			
Date	Time	16/01/2025	00:00 PM
Calibration Reference No.		SER25-010004	
Barometric Pressure		762.74	mmHg
Calibration Meter Gamma		1.001	

Factors/Conversions		
Std Temp	293	K
Std Press	760	mm Hg
K ₁	0.386	
Console Leak Check	PASS	

Calibration Data									
Run Time	Metering Console					Calibration Meter			
Elapsed	DGM Orifice DH	Volume Initial	Volume Final	Outlet Temp Initial	Outlet Temp Final	Volume Initial	Volume Final	Outlet Temp Initial	Outlet Temp Final
(Q)	(P _m)	(V _{mi})	(V _{mf})	(t _{mi})	(t _{mf})	(V _{wi})	(V _{wf})	(t _{wi})	(t _{wf})
min	mm H ₂ O	m ³	m ³	°C	°C	m ³	m ³	°C	°C
12.05	13.0	465.0450	465.1850	28	28	271.11340	271.25016	27	27
12.10	13.0	465.1850	465.3250	28	28	271.25016	271.38674	26	26
8.47	26.0	465.3320	465.4720	29	29	271.39350	271.52950	26	26
8.47	26.0	465.4720	465.6120	29	29	271.52950	271.66582	26	26
13.80	40.0	465.6240	465.9090	30	30	271.67428	271.95262	25	25
13.77	40.0	465.9040	466.1840	31	31	271.95262	272.22790	25	25
10.28	70.0	466.4960	466.7760	31	31	272.23430	272.50876	25	25
10.27	70.0	466.4760	466.7560	31	31	272.50876	272.78342	24	24
9.08	90.0	466.7690	467.0490	31	31	272.78958	273.06338	24	24
9.07	90.0	467.0490	467.3290	31	31	273.06338	273.33728	24	24



**METHOD 5 CONSOLE CALIBRATION
USING REFERENCE WET GAS METER W-NK-2.5-B-Z No.547425
5-POINT METRIC UNIT**

Meter Console Information	
Console Model Number	XC-572-V
Console Serial Number	0803018
DGM Model Number	SK25EX
DGM Serial Number	00009766

Calibration Conditions			
Date	Time	16/01/2025	00:00 PM
Calibration Reference No.		SER25-010004	
Barometric Pressure		762.74	mmHg
Calibration Meter Gamma		1.001	

Factors/Conversions		
Std Temp	293	K
Std Press	760	mm Hg
K ₁	0.386	
Console Leak Check		PASS

Calibration Data								
Results								
Standardized Data				Dry Gas Meter				
Dry Gas Meter		Calibration Meter		Calibration Factor		Flowrate	.0212 m ³ _{std} /min	Variation
(V _{m(std)})	(Q _{m(std)})	(V _{w(std)})	(Q _{w(std)})	Value	Variation	Std & Corr		
m ³	m ³ /min	m ³	m ³ /min	(Y)	(ΔY)	(Q _{m(std)(corr)})	(ΔH _@)	(ΔH _@)
						m ³ /min	mm H ₂ O	
0.137	0.011	0.134	0.011	0.977	0.003	0.011	46.452	0.575
0.138	0.011	0.134	0.011	0.975	0.001	0.011	46.805	0.928
0.138	0.016	0.134	0.016	0.970	-0.004	0.016	46.340	0.463
0.138	0.016	0.134	0.016	0.972	-0.002	0.016	46.123	0.246
0.282	0.020	0.275	0.020	0.974	0.000	0.020	45.188	-0.689
0.277	0.020	0.272	0.020	0.980	0.006	0.020	45.975	0.098
0.278	0.027	0.271	0.026	0.975	0.001	0.026	45.421	-0.456
0.279	0.027	0.272	0.027	0.975	0.001	0.027	45.056	-0.821
0.280	0.031	0.271	0.030	0.970	-0.004	0.030	45.806	-0.071
0.280	0.031	0.271	0.030	0.971	-0.003	0.030	45.604	-0.273
				0.974	Y Average		45.877	ΔH _@ Average

Note: For Calibration Factor Y, the ratio of the reading of the calibration meter to the dry gas meter, acceptable tolerance of individual values from the average is ±0.02.

For ΔH_@, orifice pressure differential that equates to 0.75 cfm (0.0212 m³/min) at standard temperature and pressure, acceptable tolerance of individual values from the average is ±0.2 inches (5.1mm) H₂O.




เอกสารไมควบคุม

Meter Console Information	
Console Model Number	XC-572-V
Console Serial Number	0803018
DGM Model Number	SK25EX
DGM Serial Number	00009766

Calibration Conditions			
Date	Time	16/01/2025	00:00 PM
Calibration Reference No.		SER25-010004	
Barometric Pressure		762.74	mmHg
Calibration Meter Gamma		1.001	

Factors/Conversions		
Std Temp	293	K
Std Press	760	mm Hg
K ₁	0.386	
Console Leak Check		PASS

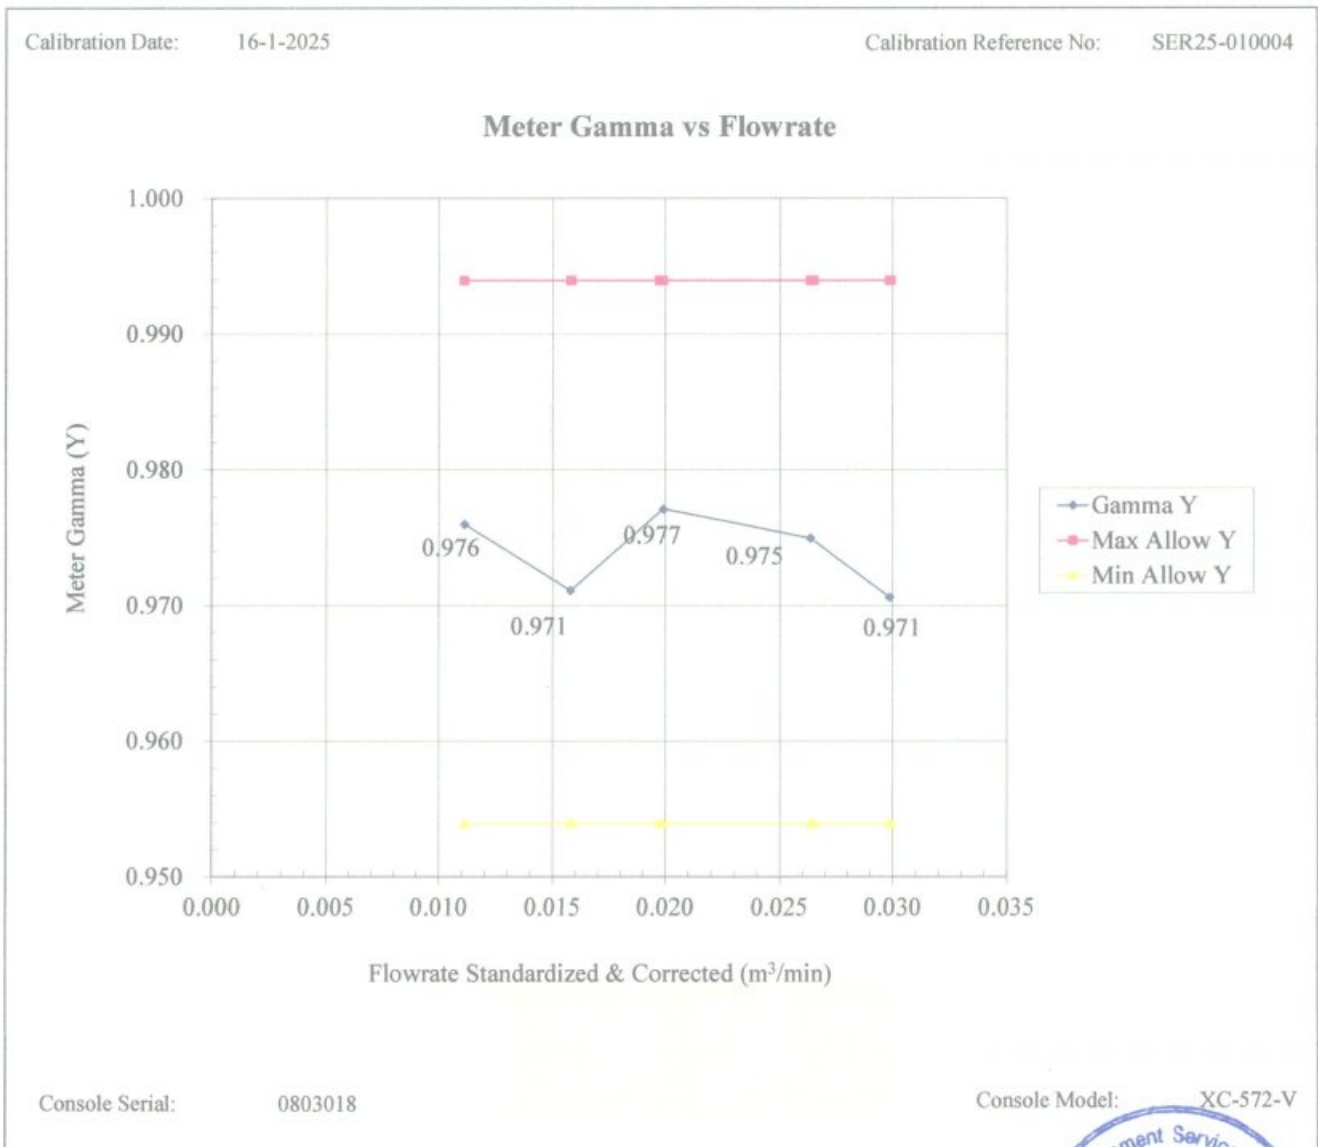

เอกสารไม่ควบคุม

Meter Console Information	
Console Model Number	XC-572-V
Console Serial Number	0803018
DGM Model Number	SK25EX
DGM Serial Number	00009766


Calibration Conditions			
Date	Time	16/01/2025	00:00 PM
Calibration Reference No.		SER25-010004	
Barometric Pressure		762.74	mmHg
Calibration Meter Gamma		1.001	

Factors/Conversions		
Std Temp	293	K
Std Press	760	mm Hg
K ₁	0.386	
Console Leak Check	PASS	

Calibration Date: 16-1-2025

Calibration Reference No: SER25-010004

Meter Pressure vs Flowrate

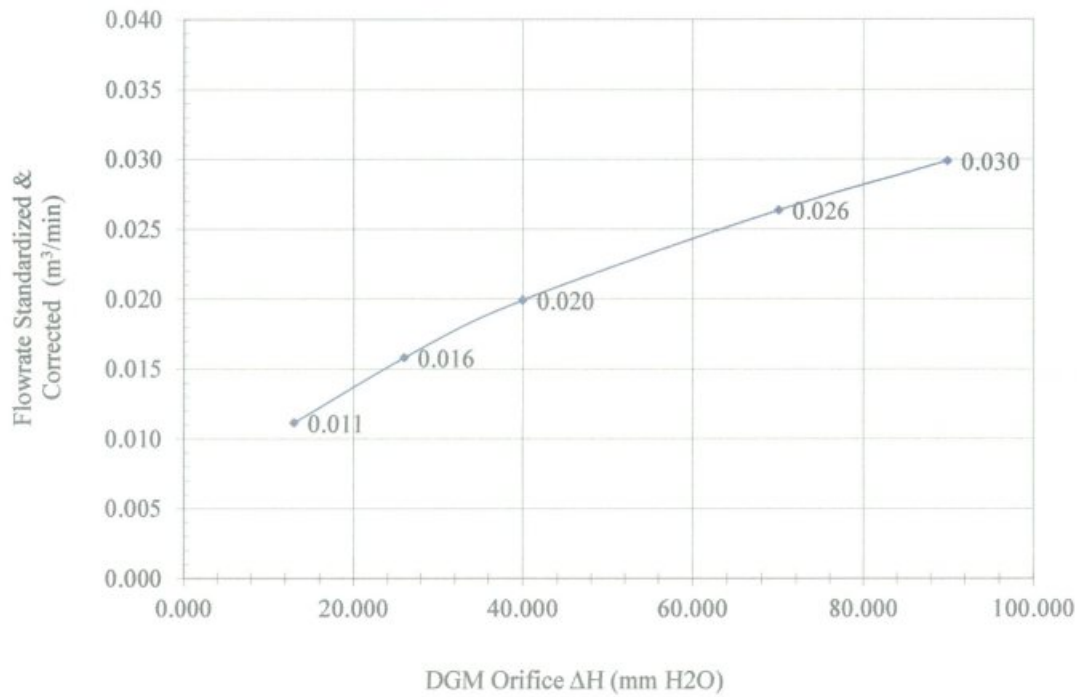

Console Serial: 0803018

Console Model: XC-572-V



เอกสารไม่ควบคุม

THERMOCOUPLES SYSTEM CALIBRATION

Sampling System Equipment Information	
Console Model Number	XC-572-V
Console Serial Number	0803018
DGM Model Number	SK25EX
DGM Serial Number	00009766
Meter Box Model Number	JENCO 765 KF
Meter Box Serial Number	JC 16095

Calibration Conditions			
Date	Time	16/01/2025	02:20 PM
Calibration Reference No.		SER25-010004	
Reference Thermometer		DIGICON	
Serial Number		183169105	

Results											
Console Thermocouple Simulator											
Channel and test point	Meter Box Channel Temperature Reading (°C)										
	-18.0	25.0	38.0	93.0	149.0	260.0	371.0	482.0	593.0	816.0	1038.0
Stack	-17.0	24.0	37.0	93.0	149.0	258.0	371.0	481.0	592.0	814.0	1037.0
Aux	-17.0	24.0	37.0	93.0	149.0						
Probe	-17.0	24.0	37.0	93.0	149.0						
Filter	-17.0	24.0	37.0	93.0	149.0						
Oven	-	-	-	-	-						
Exit	-17.0	24.0	37.0								

Tolerance Range

Stack ± 1.50% Absolute
 Probe ± 3.0 °C
 Filter ± 3.0 °C

Meter ± 3.0 °C
 Exit ± 2.0 °C



เอกสารไมควบคุม

Certificate No: G 680378

Date of issue : 12-Jun-25

Instrument description : Flue Gas Analyzer
Instrument model : Testo 350 New
Instrument serial no. : 62289477/0420
Control unit serial no. : 03498307/0420
ID no. or control no. : UAE.EFM.090/2563
Manufacturer : Testo SE & Co. KGaA
Probe description : -
Probe model : -
Probe serial no. : -
Customer name : United Analyst and Engineering Consultant Co.,Ltd.
Customer address : 81 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260

Total pages of certificate : 2 Pages
Receiving no. : L-252038
Receiving date. : 05-Jun-25
Parameter of calibration : Gas Calibration(Oxygen 2.50, 9.984, 21.01 %vol, Carbon Monoxide 80.45, 302, 1007 ppm, Nitrogen Dioxide 30.68, 81.8, 202.6 ppm, Nitric Oxide 30.0, 151.8, 322.5 ppm, Sulphur Dioxide 50.36, 100.7 ,600.8 ppm, Carbon dioxide 39.9 %Vol)
Condition of UUC. : Used
Ambient condition : All of the Measurement were carried out the stabilized labotary
 Temperature : 23 ±5 °C
 Humidity : 55 ± 15 %RH
Calibration place : 17/121 Soi Ngamwongwan 47 Yaek 48, Toongsonghong, Laksi, Bangkok 10210
Calibration procedure no : This instrument was calibrated by comparison with Standard gas mixture according to calibration Work Instruction no. WI-CL-28-C

The calibration certificate expanded uncertainty of measurement is stated as the standard uncertainty of measurent Multiplied by coverage factor $k=2$, which for a normal distribution corresponds to a coverage probability of approximately 95%.

This certificate is applied only to item under test Environmental condition.

This Calibration Certificate may not be reporduced other than in full except with the permission of the issuing laboratory. Calibration certificates without signature and seal not valid and The results relate only to the items tested/calibrated.

This calibration certificate documents are traceability to national standards, which realize measurement according to the International System of Units (SI).

Date of calibration : 12-Jun-25

Mr. Kwanchai Khamdoung

Calibration Technician

Mrs. Nongluck Wongsettee

Technical Manager

Certificate No.: G 680378

Standard References (Table 1)

Standard	Certificate No.	Vendor	Due date
Oxygen (O ₂) 2.50 % Vol	2412/23	Linde	27-Aug-27
Oxygen (O ₂) 9.984 % Vol	CG-0113-24	Nimt	01-Aug-29
Oxygen (O ₂) 21.01 % Vol	CG-0112-24	Nimt	01-Aug-29
Carbon monoxide (CO) 80.45 ppm	CG-0132-24	Nimt	10-Sep-29
Carbon monoxide (CO) 302 ppm	1915/23	Linde	16-Jun-25
Carbon monoxide (CO) 1007 ppm	1870/24	Linde	17-Jun-26
Nitrogen Dioxide (NO ₂) 30.68 ppm	2832/24	Linde	08-Sep-26
Nitrogen Dioxide (NO ₂) 81.8 ppm	2330/24	Linde	01-Aug-26
Nitrogen Dioxide (NO ₂) 202.6 ppm	3794/24	Linde	23-Dec-26
Nitric Oxide (NO) 30.0 ppm	CG-0065-24	Nimt	06-May-26
Nitric Oxide (NO) 151.8 ppm	0404/25	Linde	09-Feb-27
Nitric Oxide (NO) 322.5 ppm	1974/23	Linde	17-Jul-25
Sulphur Dioxide (SO ₂) 50.36 ppm	2004/23	Linde	17-Jul-25
Sulphur Dioxide (SO ₂) 100.7 ppm	2662/24	Linde	25-Aug-26
Sulphur Dioxide (SO ₂) 600.8 ppm	2003/23	Linde	17-Jul-25
Carbon dioxide (CO ₂) 39.9 %Vol	3508/24	Linde	07-Nov-28

Measured room conditions

Temperature : 23.3 °C Humidity : 65.2 %RH Pressure : 1010.1 mbar

Calibration conditions

Gas Temperature : 23 °C Flow rate : 1,300 ml/min Gas pressure : 1015.8 mbar

Calibration Results (Without adjustment) (Table 2)

Parameter of Standard	Standard Values	Mean of UUC	Error	Uncertainty (±)
O ₂ (%Vol)	2.50	2.52	0.02	0.15
O ₂ (%Vol)	9.984	10.09	0.106	0.20
O ₂ (%Vol)	21.01	21.13	0.12	0.30
CO (ppm)	80.45	81	0.55	3.0
CO (ppm)	302	303	1	6.0
CO (ppm)	1007	1007	0	12
NO ₂ (ppm)	30.68	28.9	-1.78	8.0
NO ₂ (ppm)	81.8	80.1	-1.7	8.0
NO ₂ (ppm)	202.6	199.7	-2.9	12
NO (ppm)	30.0	29	-1.0	8.0
NO (ppm)	151.8	153	1.2	8.0
NO (ppm)	322.5	321	-1.5	12
SO ₂ (ppm)	50.36	50	-0.36	6.0
SO ₂ (ppm)	100.7	101	0.3	6.0
SO ₂ (ppm)	600.8	600	-0.8	13
*CO ₂ (%Vol)	39.9	40.25	0.35	0.40

Remark : 1 cmol/mol = 1 %vol, 1 μmol/mol = 1 ppm., Sensor (CO,CO₂) New.

* Calibrations marked Not TISI Accredited "in this Certificate have been included for completeness."

End of Report

ขอมอบประกาศนียบัตรนี้เพื่อแสดงว่า

นายอภิวิชญ์ ท่วงที

ได้ผ่านการฝึกอบรมและทดสอบผู้ตรวจวัดความทึบแสงของเขม่าควันด้วยสายตา
และการใช้แผนภูมิเขม่าควันของริงเกิลมานน์

ระหว่างวันที่ ๑๒ - ๑๓ มีนาคม ๒๕๕๘

จัดโดย สำนักจัดการคุณภาพอากาศและเสียง กรมควบคุมมลพิษ

ให้ไว้ ณ วันที่ ๑๓ มีนาคม ๒๕๕๘

กรมควบคุมมลพิษ

(นายวิเชียร จุ่งรุ่งเรือง)

POLLUTION CONTROL DEPARTMENT

อธิบดีกรมควบคุมมลพิษ



ขอมอบประกาศนียบัตรนี้เพื่อแสดงว่า

นายนภสินธุ์ ธนุธรรมรัตน์

ได้ผ่านกำหนดการฝึกอบรมและทดสอบผู้ตรวจวัดความทึบแสงของเขม่าควันด้วยสายตา
และการใช้แผนภูมิเขม่าควันของริงเกิลมานน์ ประจำปีงบประมาณ ๒๕๖๐

ระหว่างวันที่ ๓๐ - ๓๑ มีนาคม ๒๕๖๐

จัดโดย สำนักจัดการคุณภาพอากาศและเสียง กรมควบคุมมลพิษ
ให้ไว้ ณ วันที่ ๓๑ มีนาคม ๒๕๖๐

(นายจตุพร บุรุษพัฒน์)
อธิบดีกรมควบคุมมลพิษ



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL.0-2717-3000-29 FAX.0-2719-9484



Certificate of Calibration

Cert.No.: 25CH22
Page.: 1 of 3

Equipment : pH Meter
Manufacturer : Horiba
Model : LAQUA-PH210
Serial No. : HA0F0026
ID No. : UAE.EFM.068/2564(EFM.pH.01/64)
Condition As-Received: Used Item
Received Date : 08 January 2025
Calibration Date : 09 January 2025
Reference : 2501-0223WSC-1
Submitted by : United Analyst and Engineering Consultant Co.,Ltd.
3 Soi Udomsuk 41, Sukhumvit Road,
Bangchak, Phrakhanong, Bangkok 10260
Ambient Temperature : (25 ± 2.5) °C
Relative Humidity : (50 ± 15) %
Calibration Procedure : In - house method :
- CP-CH5 by direct measurement with DC voltage standard and direct measurement with certified reference material (CRM)
- CP-CH8 by comparison with temperature standard
Calibrated by : Warakorn Lerngagtrakul
Approved by : 
Approved Signatory
 Pornthippa Tameyakul
 Ponpan Paipim
 Saithip Meangmai
Issue Date : 10 January 2025

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

เอกสารไม่ควบคุม



Cert.No.: 25CH22
Page.: 2 of 3

Condition of this calibration result

1. Reference Standard Instrument

<u>Instrument</u>	<u>Serial No.</u>	<u>ID No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
1)Document Process Calibrator	54030049	130RC116	24E2759	25 Aug 2025
2)Ref. Standard Thermometer	4982054	110RC044	24I757	14 July 2025

- This Certification is traceable to SI Through Technology Promotion Association (Thailand - Japan)

2. Certified Reference Materials :The measurement results are traceable to SI through Hach Lenge GmbH Ltd.,
Deutsche Akkreditierungsstelle, Accredited No.D-RM-15184-01-00

:The measurement results are traceable to SI through CPA chem Ltd.,
ANSI-ASQ National Accreditation Board, Accredited No. AR-1835

<u>Buffer Solution</u>	<u>Manufacturer</u>	<u>Lot No.</u>	<u>Exp. date</u>
pH 4.008	CPA chem	1034203	27 Sep 2026
pH 7.000	Hach Lenge GmbH	C03185	09 July 2026
pH 10.010	CPA chem	1034205	27 Sep 2025

3. This certificate is valid only to the item calibrated on date and place of calibration.

Calibration Results

Function : mV Measurement

Performing standard curve by Document Process Calibrator at pH (4,7)(7,10)

Unit Under Calibration	Nominal Value	Standard Voltage Input	Actual Reading		Uncertainty of Measurement (±mV)	Coverage factor <i>k</i>
	pH	mV	mV	pH		
pH Meter S/N.: HA0F0026	4.00	177.48	177.5	4.01	0.058	2.00
	7.00	0.00	0.1	7.00	0.058	2.00
	7.00	0.00	0.1	7.00	0.058	2.00
	10.00	-177.48	-177.3	10.01	0.058	2.00

**Calibration Results****Function : pH Measurement**

Performing three buffers standard curve by using buffer nominal pH (4,7)(7,10)

Unit Under Calibration	Standard pH Buffer Solution	Actual pH Reading	Actual mV Reading (mV)	Uncertainty of pH Measurement (\pm)	Coverage factor k
pH Electrode S/N.: -	4.008	4.01	186.1	0.0071	2.00
	7.000	7.00	10.2	0.0095	2.00
	7.000	7.00	10.0	0.0095	2.00
	10.010	10.01	-164.3	0.0092	2.00

Function : Temperature Measurement**(*) Without adjustment**

This equipment was connected with Temperature Probe;

- Model : _____ -

- Serial No. : _____ -

Dimension of probe

- Length : 104 mm.

- Diameter : 16 mm.

- Immersion Depth : 90 mm.

Calibration Point (°C)	Standard Temperature (°C)	UUC* Reading (°C)	Error (°C)	Uncertainty of measurement (\pm °C)	Coverage factor k
15.0	15.002	15.0	-0.002	0.13	2.00
30.0	30.002	30.0	-0.002	0.13	2.00
45.0	45.004	45.0	-0.004	0.13	2.00

Remark - UUC* = Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k , providing a level of confidence of approximately 95 %.

-o0o-



Certificate of Calibration

Cert.No.: 25CH53

Page.: 1 of 3

Equipment :	Conductivity Meter
Manufacturer :	Horiba
Model :	LAQUA-EC210
Serial No. :	HC0J0015
ID No. :	UAE.EFM.075/2564(EFM.SCT.01/64)
Condition As-Received:	Used Item
Received Date :	14 January 2025
Calibration Date :	15 January 2025
Reference :	2501-0475WSC-1
Submitted by :	United Analyst and Engineering Consultant Co.,Ltd. 3 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Ambient Temperature :	(25 ± 2.5) °C
Relative Humidity :	(50 ± 15) %
Calibration Procedure:	In -house method : - CP-CH6 by direct measurement with certified reference material (CRM) - CP-CH8 by comparison with temperature standard
Calibrated by :	Warakorn Lergagtrakul
Approved by :	<hr/> Approved Signatory
() Pornthippa Tameyakul	
() Ponpan Paipim	
(✓) Saithip Meangmai	
Issue Date :	17 January 2025

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

เอกสารไม่ควบคุม



Cert.No.: 25CH53

Page.: 2 of 3

Condition of this result of calibration

1. Reference Standard Instrument :-

<u>Instrument</u>	<u>Serial No.</u>	<u>ID No.</u>	<u>Certificate No.</u>	<u>Due date</u>
1) Thermometer	1963878	130RC095	24I995	09 Sep 2025
2) Ref. Std.Thermometer	4982054	110RC044	24I757	14 July 2025

- This Certification is traceable to SI Through Technology Promotion Association (Thailand - Japan)

2. Certified Reference Materials :-

- Conductivity calibration solution, CPA chem Ltd., The measurement results are traceable to SI through CPA chem Ltd., ANSI-ASQ National Accreditation Board, Accredited No. AR-1835

<u>Conductivity Solution</u>	<u>Manufacturer</u>	<u>Lot No.</u>	<u>Exp. date</u>
1412.9 μ S/cm	CPA Chem	1005307	15 June 2025
12.881 mS/cm	CPA Chem	1005308	15 June 2025

- Control Conductivity calibration solution temperature by Water bath (25 ± 0.1) °C

3. This certificate is valid only to the item calibrated on date and place of calibration.

Calibration results

Function : Conductivity Measurement

(*) After Adjustment at 1412.9 μ S/cm

Conductivity Electrode Serial No.: 9B0K0156

Standard Conductivity Solution	Before Adjustment UUC* Reading	After Adjustment UUC* Reading	Uncertainty of Measurement (\pm)	Coverage factor <i>k</i>
1412.9 μ S/cm	1406 μ S/cm	1413 μ S/cm	9.2 μ S/cm	2.00
12.881 mS/cm	12.45 mS/cm	12.59 mS/cm	0.086 mS/cm	2.00

Remark : - UUC* = Unit Under Calibration



Cert.No.: 25CH53

Page.: 3 of 3

Calibration Results

Function : Temperature Measurement

This equipment was connected with Temperature Probe;

- Model : 9383
- Serial No. : 9B0K0156

Dimension of probe;

- Length : 110 mm
- Diameter : 16 mm
- Immersion Depth : 100 mm

Calibration Result : Without adjustment

Calibration Point (°C)	Standard Temperature (°C)	UUC* Reading (°C)	Error (°C)	Uncertainty of Measurement (± °C)	Coverage factor <i>k</i>
15.0	15.002	15.0	-0.002	0.13	2.00
30.0	30.004	30.0	-0.004	0.13	2.00
45.0	45.002	45.1	0.098	0.13	2.00

Remark : - UUC* = Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

Envi Equipment Service Co., Ltd.

110/254 Moo 3, Tumbon Bang Rak Phatthana, Amphur Bang Bua Thong, Nonthaburi 11110

Tel. 098 362 9152, 089 478 7885

E-mail: sales@envi-ees.com

Certificate No.: E25-010007

Page: 1 of 6

CERTIFICATE OF CALIBRATION

Customer : United Analyst and Engineering Consultant Co., Ltd.
 Address : 81 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
 Description of Equipment : Console meter
 Manufacturer : Apex Instrument
 Model Number : XC-572-V
 Serial Number : 0803018
 ID./Control No. : UAE.ANV.193/2551
 Environment Conditions : Temperature (25 ± 2) °C
 : Humidity (50 ± 15) % RH
 Cal. Date : 16/01/2025
 Issue Date : 16/01/2025

Calibration Method or Calibration Procedure Used

US EPA Method (United State Environmental Protection Agency)

This certificate is traceable to national standard, which realize the units of measurement according to the International System of Units (IS).

Result of Calibration

This certificate may not be reproduced other than in full except with prior Written approval of the Technical Manager, Envi Equipment Service Company Limited.

These reported uncertainties of measurement are expanded by a coverage factor of k=2, providing a 95% confidence level

Calibrated by : Mr. Sanya Sangnil

Approved by : 
 (Mr. Mana Fuched)

Technical Manger

เอกสารไมคอบคุม



Certificate No. : E25-010007

Page : 2 of 6

**METHOD 5 CONSOLE CALIBRATION
 USING REFERENCE WET GAS METER W-NK-2.5-B-Z No.547425
 5-POINT METRIC UNIT**

Meter Console Information		Calibration Conditions				Factors/Conversions		
Console Model Number	XC-572-V	Date	Time	16/01/2025	00:00 PM	Std Temp	293	K
Console Serial Number	0803018	Calibration Reference No.	SER25-010004			Std Press	760	mm Hg
DGM Model Number	SK25EX	Barometric Pressure	762.74		mmHg	K ₁	0.386	
DGM Serial Number	00009766	Calibration Meter Gamma	1.001			Console Leak Check	PASS	

Calibration Data									
Run Time	Metering Console					Calibration Meter			
	DGM Orifice DH	Volume Initial	Volume Final	Outlet Temp Initial	Outlet Temp Final	Volume Initial	Volume Final	Outlet Temp Initial	Outlet Temp Final
Elapsed (Q)	(P _n) mm H ₂ O	(V _m) m ³	(V _{mf}) m ³	(t _{mi}) °C	(t _{mf}) °C	(V _{wi}) m ³	(V _{wf}) m ³	(t _{wi}) °C	(t _{wf}) °C
min	mm H ₂ O	m ³	m ³	°C	°C	m ³	m ³	°C	°C
12.05	13.0	465.0450	465.1850	28	28	271.11340	271.25016	27	27
12.10	13.0	465.1850	465.3250	28	28	271.25016	271.38674	26	26
8.47	26.0	465.3320	465.4720	29	29	271.39350	271.52950	26	26
8.47	26.0	465.4720	465.6120	29	29	271.52950	271.66582	26	26
13.80	40.0	465.6240	465.9090	30	30	271.67428	271.95262	25	25
13.77	40.0	465.9040	466.1840	31	31	271.95262	272.22790	25	25
10.28	70.0	466.4960	466.7760	31	31	272.23430	272.50876	25	25
10.27	70.0	466.4760	466.7560	31	31	272.50876	272.78342	24	24
9.08	90.0	466.7690	467.0490	31	31	272.78958	273.06338	24	24
9.07	90.0	467.0490	467.3290	31	31	273.06338	273.33728	24	24



เอกสารไมคอบคุม

METHOD 5 CONSOLE CALIBRATION
USING REFERENCE WET GAS METER W-NK-2.5-B-Z No.547425
5-POINT METRIC UNIT

Meter Console Information		Calibration Conditions				Factors/Conversions		
Console Model Number	XC-572-V	Date	Time	16/01/2025	00:00 PM	Std Temp	293	K
Console Serial Number	0803018	Calibration Reference No.	SER25-010004			Std Press	760	mm Hg
DGM Model Number	SK25EX	Barometric Pressure	762.74			K ₁	0.386	
DGM Serial Number	00009766	Calibration Meter Gamma	1.001			Console Leak Check	PASS	


Calibration Data									
Results									
Standardized Data				Dry Gas Meter					
Dry Gas Meter		Calibration Meter		Calibration Factor		Flowrate			
(V _{m(std)})	(Q _{m(std)})	(V _{w(std)})	(Q _{w(std)})	Value	Variation	Std & Corr	.0212 m ³ _{std} /min	Variation	
m ³	m ³ /min	m ³	m ³ /min	(Y)	(ΔY)	(Q _{m(std)corr})	(ΔH _g)	(ΔH _g)	
						m ³ /min	mm H ₂ O		
0.137	0.011	0.134	0.011	0.977	0.003	0.011	46.452	0.575	
0.138	0.011	0.134	0.011	0.975	0.001	0.011	46.805	0.928	
0.138	0.016	0.134	0.016	0.970	-0.004	0.016	46.340	0.463	
0.138	0.016	0.134	0.016	0.972	-0.002	0.016	46.123	0.246	
0.282	0.020	0.275	0.020	0.974	0.000	0.020	45.188	-0.689	
0.277	0.020	0.272	0.020	0.980	0.006	0.020	45.975	0.098	
0.278	0.027	0.271	0.026	0.975	0.001	0.026	45.421	-0.456	
0.279	0.027	0.272	0.027	0.975	0.001	0.027	45.056	-0.821	
0.280	0.031	0.271	0.030	0.970	-0.004	0.030	45.806	-0.071	
0.280	0.031	0.271	0.030	0.971	-0.003	0.030	45.604	-0.273	
				0.974	Y Average			45.877	ΔH@ Average

Note: For Calibration Factor Y, the ratio of the reading of the calibration meter to the dry gas meter, acceptable tolerance of individual values from the average is ±0.02.
For ΔH_g, orifice pressure differential that equates to 0.75 cfm (0.0212 m³/min) at standard temperature and pressure, acceptable tolerance of individual values from the average is ±0.2 inches (5.1mm)



เอกสารไม่ควบคุม

Meter Console Information		Calibration Conditions				Factors/Conversions		
Console Model Number	XC-572-V	Date	Time	16/01/2025	00:00 PM	Std Temp	293	K
Console Serial Number	0803018	Calibration Reference No.	SER25-010004			Std Press	760	mm Hg
DGM Model Number	SK25EX	Barometric Pressure	762.74			K ₁	0.386	
DGM Serial Number	00009766	Calibration Meter Gamma	1.001			Console Leak Check	PASS	

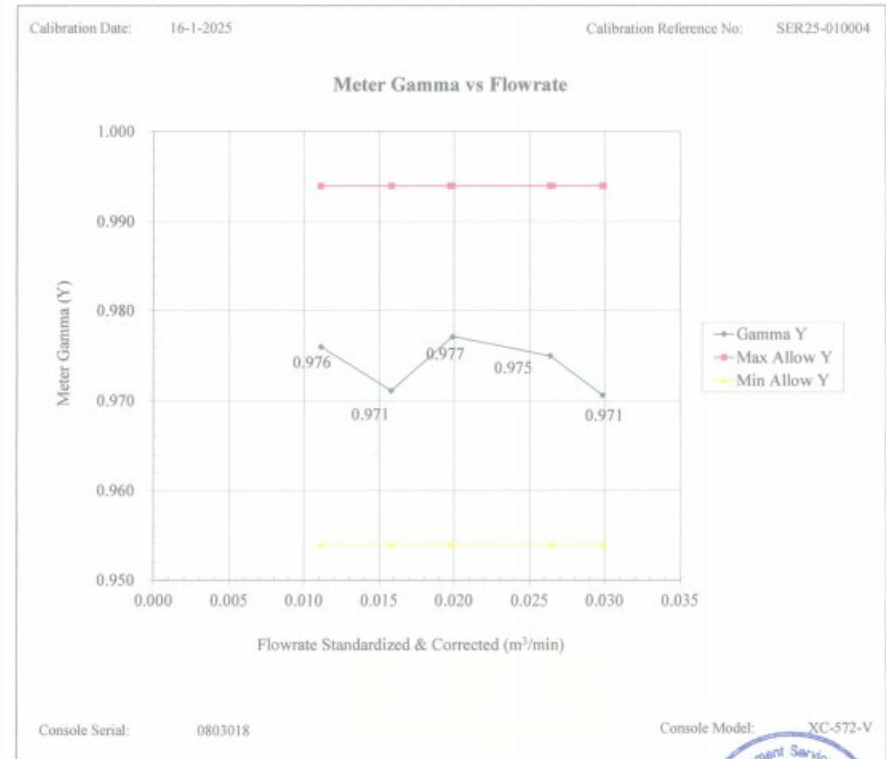

เอกสารไม่ควบคุม


Meter Console Information	
Console Model Number	XC-572-V
Console Serial Number	0803018
DGM Model Number	SK25EX
DGM Serial Number	00009766

Calibration Conditions			
Date	Time	16/01/2025	00:00 PM
Calibration Reference No.	SER25-010004		
Barometric Pressure	762.74	mm Hg	
Calibration Meter Gamma	1.001		

Factors/Conversions		
Std Temp	293	K
Std Press	760	mm Hg
K ₁	0.386	
Console Leak Check	PASS	

Calibration Date: 16-1-2025 Calibration Reference No: SER25-010004

Meter Pressure vs Flowrate

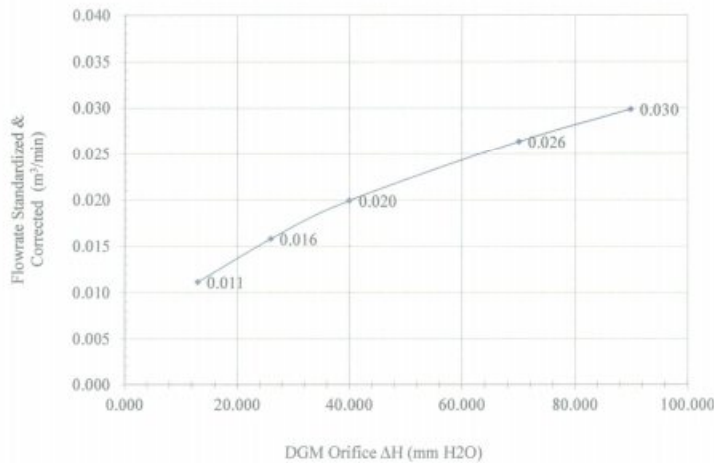

Console Serial: 0803018

Console Model: XC-572-V



เอกสารไม่ควบคุม

THERMOCOUPLES SYSTEM CALIBRATION

Sampling System Equipment Information	
Console Model Number	XC-572-V
Console Serial Number	0803018
DGM Model Number	SK25EX
DGM Serial Number	00009766
Meter Box Model Number	JENCO 765 KF
Meter Box Serial Number	JC 16095

Calibration Conditions			
Date	Time	16/01/2025	02:20 PM
Calibration Reference No.	SER25-010004		
Reference Thermometer	DIGICON		
Serial Number	183169105		

Results

Channel and test point	Console Thermocouple Simulator										
	Meter Box Channel Temperature Reading (°C)										
	-18.0	25.0	38.0	93.0	149.0	260.0	371.0	482.0	593.0	816.0	1038.0
Stack	-17.0	24.0	37.0	93.0	149.0	258.0	371.0	481.0	592.0	814.0	1037.0
Aux	-17.0	24.0	37.0	93.0	149.0						
Probe	-17.0	24.0	37.0	93.0	149.0						
Filter	-17.0	24.0	37.0	93.0	149.0						
Oven	-	-	-	-	-						
Exit	-17.0	24.0	37.0								

Tolerance Range

Stack	± 1.50%	Absolute	Meter	± 3.0 °C
Probe	± 3.0 °C		Exit	± 2.0 °C
Filter	± 3.0 °C			



เอกสารไม่ควบคุม

Certificate No.: G 680378
Date of issue : 12-Jun-25

Instrument description : Flue Gas Analyzer
Instrument model : Testo 350 New
Instrument serial no. : 62289477/0420
Control unit serial no. : 03498307/0420
ID no. or control no. : UAE.EFM.090/2563
Manufacturer : Testo SE & Co. KGaA
Probe description : -
Probe model : -
Probe serial no. : -
Customer name : United Analyst and Engineering Consultant Co.,Ltd.
Customer address : 81 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260

Total pages of certificate : 2 Pages
Receiving no. : L-252038
Receiving date. : 05-Jun-25
Parameter of calibration : Gas Calibration(Oxygen 2.50, 9.984, 21.01 %vol, Carbon Monoxide 80.45, 302, 1007 ppm, Nitrogen Dioxide 30.68, 81.8, 202.6 ppm, Nitric Oxide 30.0, 151.8, 322.5 ppm, Sulphur Dioxide 50.36, 100.7, 600.8 ppm, Carbon dioxide 39.9 %Vol)

Condition of UUC. : Used
Ambient condition : All of the Measurement were carried out the stabilized labotary
Temperature : 23 ± 5 °C
Humidity : 55 ± 15 %RH

Calibration place : 17/121 Soi Ngamwongwan 47 Yaek 48, Toongsonghong, Laksi, Bangkok 10210

Calibration procedure no. : This instrument was calibrated by comparison with Standard gas mixture according to calibration Work Instruction no. WI-CL-28-C

The calibration certificate expanded uncertainty of measurement is stated as the standard uncertainty of measurent Multiplied by coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

This certificate is applied only to item under test Environmental condition.

This Calibration Certificate may not be reproduced other than in full except with the permission of the issuing laboratory. Calibration certificates without signature and seal not valid and The results relate only to the items tested/calibrated.

This calibration certificate documents are traceability to national standards, which realize measurement according to the International System of Units (SI).

Date of calibration : 12-Jun-25



Mr. Kwanchai Khamdoug
Calibration Technician



Mrs. Nongluck Wongsettee
Technical Manager

Certificate No.: G 680378

Standard References (Table 1)

Standard	Certificate No.	Vendor	Due date
Oxygen (O2) 2.50 % Vol	2412/23	Linde	27-Aug-27
Oxygen (O2) 9.984 % Vol	CG-0113-24	Nimt	01-Aug-29
Oxygen (O2) 21.01 % Vol	CG-0112-24	Nimt	01-Aug-29
Carbon monoxide (CO) 80.45 ppm	CG-0132-24	Nimt	10-Sep-29
Carbon monoxide (CO) 302 ppm	1915/23	Linde	16-Jun-25
Carbon monoxide (CO) 1007 ppm	1870/24	Linde	17-Jun-26
Nitrogen Dioxide (NO2) 30.68 ppm	2832/24	Linde	08-Sep-26
Nitrogen Dioxide (NO2) 81.8 ppm	2330/24	Linde	01-Aug-26
Nitrogen Dioxide (NO2) 202.6 ppm	3794/24	Linde	23-Dec-26
Nitric Oxide (NO) 30.0 ppm	CG-0065-24	Nimt	06-May-26
Nitric Oxide (NO) 151.8 ppm	0404/25	Linde	09-Feb-27
Nitric Oxide (NO) 322.5 ppm	1974/23	Linde	17-Jul-25
Sulphur Dioxide (SO2) 50.36 ppm	2004/23	Linde	17-Jul-25
Sulphur Dioxide (SO2) 100.7 ppm	2662/24	Linde	25-Aug-26
Sulphur Dioxide (SO2) 600.8 ppm	2003/23	Linde	17-Jul-25
Carbon dioxide (CO2) 39.9 %Vol	3508/24	Linde	07-Nov-28

Measured room conditions

Temperature : 23.3 °C Humidity : 65.2 %RH Pressure : 1010.1 mbar

Calibration conditions

Gas Temperature : 23 °C Flow rate : 1,300 ml/min Gas pressure : 1015.8 mbar

Calibration Results (Without adjustment) (Table 2)

Parameter of Standard	Standard	Mean of	Error	Uncertainty (±)
	Values	UUC		
O2 (%Vol)	2.50	2.52	0.02	0.15
O2 (%Vol)	9.984	10.09	0.106	0.20
O2 (%Vol)	21.01	21.13	0.12	0.30
CO (ppm)	80.45	81	0.55	3.0
CO (ppm)	302	303	1	6.0
CO (ppm)	1007	1007	0	12
NO2 (ppm)	30.68	28.9	-1.78	8.0
NO2 (ppm)	81.8	80.1	-1.7	8.0
NO2 (ppm)	202.6	199.7	-2.9	12
NO (ppm)	30.0	29	-1.0	8.0
NO (ppm)	151.8	153	1.2	8.0
NO (ppm)	322.5	321	-1.5	12
SO2 (ppm)	50.36	50	-0.36	6.0
SO2 (ppm)	100.7	101	0.3	6.0
SO2 (ppm)	600.8	600	-0.8	13
*CO2 (%Vol)	39.9	40.25	0.35	0.40

Remark : 1 cmol/mol = 1 %vol. 1 µmol/mol = 1 ppm., Sensor (CO,CO2) New.

* Calibrations marked Not TISI Accredited "in this Certificate have been included for completeness."

End of Report

ขอมอบประกาศนียบัตรนี้เพื่อแสดงว่า

นายอภิวิชญ์ ท่วงที

ได้ผ่านการฝึกอบรมและทดสอบผู้ตรวจวัดความทึบแสงของเขม่าควันด้วยสายตา
และการใช้แผนภูมิเขม่าควันของริงเกิลมานน์

ระหว่างวันที่ ๑๒ - ๑๓ มีนาคม ๒๕๕๘

จัดโดย สำนักจัดการคุณภาพอากาศและเสียง กรมควบคุมมลพิษ

ให้ไว้ ณ วันที่ ๑๓ มีนาคม ๒๕๕๘


กรมควบคุมมลพิษ
POLLUTION CONTROL DEPARTMENT
(นายวีเชิร จิรุงเรือง)
อธิบดีกรมควบคุมมลพิษ



ขอมอบประกาศนียบัตรนี้เพื่อแสดงว่า


นายณภสินธุ์ ธนูธรรมรัตน์

ได้ผ่านการกำหนดการฝึกอบรมและทดสอบผู้ตรวจวัดความทึบแสงของเขม่าควันด้วยสายตา
และการใช้แผนภูมิเขม่าควันของริงเกิลมานน์ ประจำปีงบประมาณ ๒๕๖๐

ระหว่างวันที่ ๓๐ - ๓๑ มีนาคม ๒๕๖๐

จัดโดย สำนักจัดการคุณภาพอากาศและเสียง กรมควบคุมมลพิษ

ให้ไว้ ณ วันที่ ๓๑ มีนาคม ๒๕๖๐


(นายจตุพร บุรุษพัฒน์)
อธิบดีกรมควบคุมมลพิษ



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL.0-2717-3000-29 FAX.0-2719-9484



Certificate of Calibration

Cert.No.: 25CH22
Page.: 1 of 3

Equipment : pH Meter
Manufacturer : Horiba
Model : LAQUA-PH210
Serial No. : HA0F0026
ID No. : UAE.EFM.068/2564(EFM.pH.01/64)
Condition As-Received: Used Item
Received Date : 08 January 2025
Calibration Date : 09 January 2025
Reference : 2501-0223WSC-1
Submitted by : United Analyst and Engineering Consultant Co.,Ltd.
3 Soi Udomsuk 41, Sukhumvit Road,
Bangchak, Phrakhanong, Bangkok 10260

Ambient Temperature : (25 ± 2.5) °C
Relative Humidity : (50 ± 15) %
Calibration Procedure : In - house method :
- CP-CH5 by direct measurement with DC voltage standard and direct measurement with certified reference material (CRM)
- CP-CH8 by comparison with temperature standard

Calibrated by : Warakorn Lerngagtrakul


Approved Signatory

Approved by :

() Pornthippa Tameyakul
() Ponpan Paipim
(✓) Saithip Meangmai

Issue Date : 10 January 2025

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written Approval of the head of Corporate Services 3 - Equipment Calibration and Testing Services.

เอกสารไม่ควบคุม

Cert.No.: 25CH22
Page.: 2 of 3

Condition of this calibration result

1. Reference Standard Instrument

Instrument	Serial No.	ID No.	Cert. No.	Due Date
1)Document Process Calibrator	54030049	130RC116	24E2759	25 Aug 2025
2)Ref. Standard Thermometer	4982054	110RC044	24I757	14 July 2025

- This Certification is traceable to SI Through Technology Promotion Association (Thailand - Japan)

2. Certified Reference Materials :The measurement results are traceable to SI through Hach Lenge GmbH Ltd., Deutsche Akkreditierungsstelle, Accredited No.D-RM-15184-01-00

:The measurement results are traceable to SI through CPA chem Ltd., ANSI-ASQ National Accreditation Board, Accredited No. AR-1835

Buffer Solution	Manufacturer	Lot No.	Exp. date
pH 4.008	CPA chem	1034203	27 Sep 2026
pH 7.000	Hach Lenge GmbH	C03185	09 July 2026
pH 10.010	CPA chem	1034205	27 Sep 2025

3. This certificate is valid only to the item calibrated on date and place of calibration.

Calibration Results

Function : mV Measurement

Performing standard curve by Document Process Calibrator at pH (4,7)(7,10)

Unit Under Calibration	Nominal Value	Standard Voltage Input	Actual Reading		Uncertainty of Measurement (±mV)	Coverage factor k
	pH	mV	mV	pH		
pH Meter S/N.: HA0F0026	4.00	177.48	177.5	4.01	0.058	2.00
	7.00	0.00	0.1	7.00	0.058	2.00
	7.00	0.00	0.1	7.00	0.058	2.00
	10.00	-177.48	-177.3	10.01	0.058	2.00

เอกสารไม่ควบคุม



Cert.No.: 25CH22
Page.: 3 of 3

Calibration Results

Function : pH Measurement

Performing three buffers standard curve by using buffer nominal pH (4,7)(7,10)

Unit Under Calibration	Standard pH Buffer Solution	Actual pH Reading	Actual mV Reading (mV)	Uncertainty of pH Measurement (\pm)	Coverage factor <i>k</i>
pH Electrode S/N.: -	4.008	4.01	186.1	0.0071	2.00
	7.000	7.00	10.2	0.0095	2.00
	7.000	7.00	10.0	0.0095	2.00
	10.010	10.01	-164.3	0.0092	2.00

Function : Temperature Measurement

(*) Without adjustment

This equipment was connected with Temperature Probe;

- Model : _____
- Serial No. : _____

Dimension of probe

- Length : 104 mm.
- Diameter : 16 mm.
- Immersion Depth : 90 mm.

Calibration Point (°C)	Standard Temperature (°C)	UUC* Reading (°C)	Error (°C)	Uncertainty of measurement (\pm °C)	Coverage factor <i>k</i>
15.0	15.002	15.0	-0.002	0.13	2.00
30.0	30.002	30.0	-0.002	0.13	2.00
45.0	45.004	45.0	-0.004	0.13	2.00

Remark - UUC* = Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

เอกสารไม่ควบคุม



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLIANG, SUANLIANG BANGKOK 10250
TEL.0-2717-3000-29 FAX.0-2719-9484



Certificate of Calibration

Cert.No.: 25CH53
Page.: 1 of 3

Equipment : Conductivity Meter
Manufacturer : Horiba
Model : LAQUA-EC210
Serial No. : HC0J0015
ID No. : UAE.EFM.075/2564(EFM.SCT.01/64)
Condition As-Received: Used Item
Received Date : 14 January 2025
Calibration Date : 15 January 2025
Reference : 2501-0475WSC-1
Submitted by : United Analyst and Engineering Consultant Co.,Ltd.
3 Soi Udomsuk 41, Sukhumvit Road,
Bangchak, Phrakhanong, Bangkok 10260
Ambient Temperature : (25 \pm 2.5) °C
Relative Humidity : (50 \pm 15) %
Calibration Procedure: In -house method :
- CP-CH6 by direct measurement with certified reference material (CRM)
- CP-CH8 by comparison with temperature standard

Calibrated by : Warakorn Lerngagtrakul

Approved by : _____
Approved Signatory

() Pornthippa Tameyakul
() Ponpan Paipim
(✓) Saithip Meangmai

Issue Date : 17 January 2025

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

เอกสารไม่ควบคุม



Cert.No.: 25CH53

Page.: 2 of 3

Condition of this result of calibration

1. Reference Standard Instrument :-

Instrument	Serial No.	ID No.	Certificate No.	Due date
1) Thermometer	1963878	130RC095	241995	09 Sep 2025
2) Ref. Std. Thermometer	4982054	110RC044	241757	14 July 2025

- This Certification is traceable to SI Through Technology Promotion Association (Thailand - Japan)

2. Certified Reference Materials :-

- Conductivity calibration solution, CPA chem Ltd., The measurement results are traceable to SI through CPA chem Ltd., ANSI-ASQ National Accreditation Board, Accredited No. AR-1835

Conductivity Solution	Manufacturer	Lot No.	Exp. date
1412.9 μ S/cm	CPA Chem	1005307	15 June 2025
12.881 mS/cm	CPA Chem	1005308	15 June 2025

- Control Conductivity calibration solution temperature by Water bath (25 ± 0.1) °C

3. This certificate is valid only to the item calibrated on date and place of calibration.

Calibration results

Function : Conductivity Measurement

(*) After Adjustment at 1412.9 μ S/cm

Conductivity Electrode Serial No.: 9B0K0156

Standard Conductivity Solution	Before Adjustment UUC* Reading	After Adjustment UUC* Reading	Uncertainty of Measurement (\pm)	Coverage factor <i>k</i>
1412.9 μ S/cm	1406 μ S/cm	1413 μ S/cm	9.2 μ S/cm	2.00
12.881 mS/cm	12.45 mS/cm	12.59 mS/cm	0.086 mS/cm	2.00

Remark : - UUC* = Unit Under Calibration

เอกสารไม่ควบคุม



Cert.No.: 25CH53

Page.: 3 of 3

Calibration Results

Function : Temperature Measurement

This equipment was connected with Temperature Probe;

- Model :	9383
- Serial No. :	9B0K0156

Dimension of probe;

- Length :	110 mm
- Diameter :	16 mm
- Immersion Depth :	100 mm

Calibration Result : Without adjustment

Calibration Point (°C)	Standard Temperature (°C)	UUC* Reading (°C)	Error (°C)	Uncertainty of Measurement (\pm °C)	Coverage factor <i>k</i>
15.0	15.002	15.0	-0.002	0.13	2.00
30.0	30.004	30.0	-0.004	0.13	2.00
45.0	45.002	45.1	0.098	0.13	2.00

Remark : - UUC* = Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

เอกสารไม่ควบคุม

บริษัท อินทิเกรทเต็ด รีเสิร์ช เซ็นเตอร์ จำกัด



Certificate of Calibration

Equipment: Balance Certificate No.: C01243398
 Model: BSA224S-CW Issued Date: 06 November 2024
 Serial No. (or ID.): 34490341 Job No.: WO-00047130
 Manufacturer: Sartorius Page: 1 of 2
 Condition: In condition

Customer: Integrated Research Center Co.,Ltd.
 122 Moo 2, Tambol Thatoom,
 Amphur Srimahaphote, Prachinburi 25140 Thailand

Environment Condition: Temperature 24 °C ± 0.4 °C
 Humidity 60 %RH ± 3.3 %RH

Calibration Place: Double A (1991) Public Company Limited.
 (Water Laboratory IP1 (Balance Room))
 1 Moo 2, Thatoom, Srimahaphot,
 Prachinburi 25140 Thailand.

Calibration By: Mr. Piyapat Saidoung
 Calibration Date: 30 October 2024

The Method used: In-house method, CAL-WI-47, based on UKAS Lab 14

Traceability: This certificate is traceable to the SI Units maintained by National Institute of Metrology (NIMT), Thailand through DKSH Technology Co., Ltd. Certificate No. C02231944

Calibration Results:

Without Adjustment

Eccentric Error: Weight to be 1/3 or 1/2 of Maximum capacity, taken from the center of the pan as a zero reference.

Nominal Test Value		100 (g)				
Reference Points (g)						
A	B	C	D	E		
-	0.0001	0.0001	-0.0001	-0.0001		

Repeatability: Determination of the standard deviation of weighing balance., Readability 0.0001 (g)

Nominal test value (g)	Standard Deviation
20	0.00004
200	0.00006

Error of Indication from nominal or conventional mass value., Readability 0.0001 (g)

Nominal Value (g)	Conventional Mass (g)	Displayed Value (g)	Error of Indication (g)	Uncertainty (g)	k
0.1	0.10001	0.1000	0.0000	0.00011	2.04
0.2	0.20001	0.2000	0.0000	0.00011	2.04
0.5	0.50001	0.5000	0.0000	0.00011	2.04
1	1.00001	1.0000	0.0000	0.00011	2.04
2	2.00002	2.0000	0.0000	0.00011	2.04
5	5.00002	5.0000	0.0000	0.00011	2.04
10	10.00001	10.0000	0.0000	0.00011	2.04
20	20.00001	20.0000	0.0000	0.00012	2.03
50	50.00001	50.0000	0.0000	0.00013	2.02
100	100.00003	100.0000	0.0000	0.00017	2.01
200	200.00000	200.0000	0.0000	0.00030	2.00

The End of Certificate

(Mr. Piyapat Saidoung) (Mr. Adisai Maknoi)
 Person in charge Authorized signatory

This certificate is issued in the units of measurement according to the International System of Units (SI). It provides traceability of measurement to international or national standard or other recognized national standard laboratories. The measurement uncertainty stated is the expanded uncertainty which is obtained from the standard uncertainty multiplied by the coverage factor (k=2) to provide a level of confidence of approximately 95%. It is determined in accordance with the Guide to Expression of Uncertainty in Measurement (GUM). These results may be affected by deviations from specified conditions. The results relate only to the items tested, calibrated or sampled. This report shall not be reproduced except in full without approval of DKSH Technology Limited.

บริษัท ดีเคเอส อีเซีย จำกัด
 DKSH Technology Limited
 2533 ถนนพหลโยธิน แขวงจตุจักร เขตจตุจักร กรุงเทพฯ 10200
 2533 Sukhumvit Road, Bangkok, Prachinburi, Bangkok 10200
 Phone: +66 2638 7000 Email: info.calibration@dksh.com Website: www.dksh.com/scientific-thailand


บริษัท ดีเคเอส อีเซีย จำกัด
 DKSH Technology Limited
 2533 ถนนพหลโยธิน แขวงจตุจักร เขตจตุจักร กรุงเทพฯ 10200
 2533 Sukhumvit Road, Bangkok, Prachinburi, Bangkok 10200
 Phone: +66 2638 7000 Email: info.calibration@dksh.com Website: www.dksh.com/scientific-thailand

Delivering Growth - in Asia and Beyond.

CAL-FM-C01-14: 12 Sep 2022

Delivering Growth - in Asia and Beyond.

CAL-FM-C01-14: 12 Sep 2022

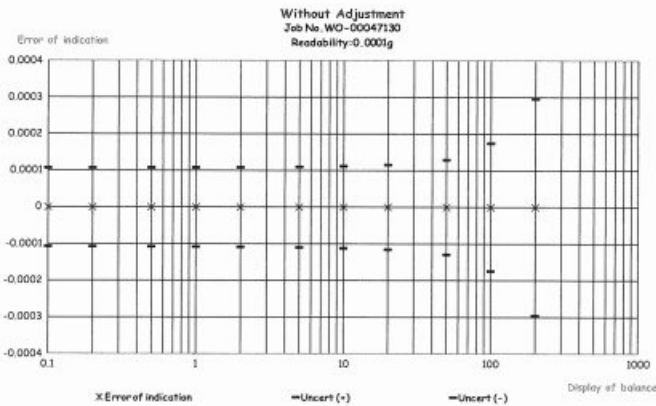

ใบตรวจสอบสภาพเครื่องชั่ง

เลขที่ใบงาน: WO-00047130

ชนิดเครื่องมือ: Balance

รุ่น: BSA224S-CW

หมายเลขเครื่อง: 34490341

ตรวจสอบ (รับ)		รายการตรวจสอบ	ตรวจสอบ (ส่ง)		หมายเหตุ
ปกติ	ไม่ปกติ		30 Oct 2024	ปกติ / ไม่ปกติ	
General					
<input checked="" type="checkbox"/>	<input type="checkbox"/>	1. สายไฟ/Adapter, power supply 220/110V	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	2. ความสมบูรณ์ชุดกรงจากกันลม (Cover)	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	3. ความสมบูรณ์ชุดชั่งระดับน้ำ	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	4. การปรับระดับของขาตั้งเครื่อง	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	5. การทดสอบของชั่งไม่ตก	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	6. ความสมบูรณ์ของ Display	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	7. การแสดงผลของ Display หลังวางน้ำหนัก	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	8. ชุดรองจานชั่ง (Stopper) / pan support	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	9. การทำงานของ Function Internal / External	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	10. ความสะอาดของตัวเครื่องภายนอกและแผ่น load cell	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	11. สภาวะแวดล้อม ณ สถานที่ตั้งเครื่อง	<input checked="" type="checkbox"/>	<input type="checkbox"/>	

หมายเหตุเพิ่มเติม/ข้อแนะนำ :

Mr. Piyapat Saidoung
 Service Engineer

บริษัท ดีเคเอส อีเซีย จำกัด
 DKSH Technology Limited
 2533 ถนนพหลโยธิน แขวงจตุจักร เขตจตุจักร กรุงเทพฯ 10200
 2533 Sukhumvit Road, Bangkok, Prachinburi, Bangkok 10200
 Phone: +66 2638 7000 Email: info.calibration@dksh.com Website: www.dksh.com/scientific-thailand

Delivering Growth - in Asia and Beyond.

CALIBRATION CERTIFICATE

Nomenclature : PERSONAL AIR PUMP SAMPLING PUMP CALIBRATION

Calibration point : (0.05, 0.5, 1, 1.5, 2) l/min

Manufacturer : MesaLabs

Ambient condition : Temperature (23 ± 3) °C , Relative humidity (55 ± 15) %

Serial No. : 210155

Atmospheric pressure (1010±13) hPa

Model : Defender 510

Calibration method : The flowmeter (UUC) was calibrated by comparison method with standard flowmeter according to CP-370.01.

Scale range : 50 ml/min to 5000 ml/min

The reported value is the value that converted to value at reference condition within pressure and temperature of the actual gas entering the UUC

Subdivision : (0.00001, 0.0001) l/min

Submitted by : INTEGRATED RESEARCH CENTER COMPANY LIMITED.

122 T.Thatoom A.Srimahaphote,

Prachinburi 25140, Thailand.

Received date : 15 January 2025 **Condition of measured item :** Normal

Calibration date : 3 February 2025

Standard	Standard	Certificate No.	Date due	Tracability
RTD Thermometer	PSL-T 0611/67	3-Jul-26	TISTR	
Molbox/Pressure Transducer/UpStream	MP-0076-23	2-Apr-25	NIMT	
Primary Flow Calibrator S/N 119521	MW-0033-23	6-Jun-25	NIMT	

Calibrated by :
(Mr.Terasak Panna)

Approved by :
(Ms.Kirana Luangniran)
Director
Mechanical Engineering Standards Laboratory

Ref. 2013268011500202001

Issued Date 5 February 2025

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

Head Office
33 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9009

Office/Laboratory
668 Mu 2 Tambon Bangpooai, Amphoe Muang Samutprakan,
Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2325 1672-80 ext. 115, 116
(66) 08 3219 9400
E-mail : mtc@tistr.or.th Website : www.tistr.or.th

Office
196 Phahonyothin Road, Ladysao, Chatuchak,
Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827

FM.BLMTC.002 Rev.5

Head Office
33 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9009

Office/Laboratory
668 Mu 2 Tambon Bangpooai, Amphoe Muang Samutprakan,
Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2325 1672-80 ext. 115, 116
(66) 08 3219 9400
E-mail : mtc@tistr.or.th Website : www.tistr.or.th

Office
196 Phahonyothin Road, Ladysao, Chatuchak,
Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827

FM.BLMTC.002 Rev.5



JIRANATEE ASSOCIATES CO.,LTD.

Jiranatee Associates Co., Ltd.
63/34-15, 47/35-16,
Hothikraem 7/21, Rd. Wathayapa, Bangkoksk,
Bangkok 10600 (Thailand)
Tel. +6628626212
Mobile: +6623090413
E-mail: jnac-cal@jiranatee.com
Web site: www.jiranatee.com

Accredited calibration laboratory
ISO/IEC 17025:2017
NSC-TSI-715-17025
CALIBRATION 0367



NSC - TSI - TIS 17025
CALIBRATION 0367

Flow measurement laboratory
Calibration services department



JIRANATEE ASSOCIATES CO.,LTD.

Continuation of Certificate of Calibration Number COF-013-67

Page 2 of 2 Pages

CERTIFICATE OF CALIBRATION

Certificate No. : COF-013-67

Page 1 of 2 Pages

MEASUREMENT ITEM : Top Load Orifice
MANUFACTURER : TSI/CI
MODEL/TYPE : 16-5028A
SERIAL NUMBER : 2926
ID NUMBER : -
CONDITION AS-RECEIVED : Used Item
CUSTOMER : Integrated Research Center Company Limited,
122 Moo 2, Thatoom, Srimahaphote,
Prachinburi 25140, Thailand.
RECEIVED DATE : 10 May 2024
MEASUREMENT DATE : 05 Jun 2024
ISSUE DATE : 06 Jun 2024

ENVIRONMENTAL CONDITIONS:
Ambient condition in the laboratory are as follow:
Temperature : 23.0 ± 3.0 °C
Relative Humidity : 55.0 ± 15.0 %RH
Atmospheric Pressure : 1010 ± 10 hPa

CALIBRATION CONDITION:
Preconditioning : 24 hours at ambient conditions.
Measurement Condition : The average values during measurement are 22.9 °C and 53.2 %RH.

NOTE: The certificate is valid only to the item calibrated on date and place of calibration.

TABULATION OF RESULTS:
The table on next page give the measured values.

Calibration procedure:
The Orifice gas flow device was calibrated against Standard Rotary Displacement Meter (Roots Meter) Model G65/MC/W2 up. The MP-CL-004 was used as a calibration guideline.

Traceability:
This certificate provides a traceability of the measurement to realization of the international system of units (SI) through the NIMT (National Metrology Institute of Thailand) via Certificate number: MW0063-23.

Uncertainty of Measurement:
The reported uncertainty of measurement is based on the standard uncertainty multiplied by a coverage factor k=2. Which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty has been determined in accordance with the GUM (Evaluation of measurement data - Guide to the expression of uncertainty in measurement)

MEASUREMENT RESULTS:

The Orifice gas flow device was calibrated by direct comparison method with the Standard Rotary Displacement Meter (Roots Meter). The humid air was used as a medium in the system. The standard conditions are 25 °C (298.15 K) and 760 mmHg for standard temperature and standard pressure respectively.

Table 1: The results of Q Standard calibration data

Rate	Flow rate m ³ /min	Pressure [Pa] mmHg	Temperature [T _a] °C	Temperature [T _m] °C	Ap_meter mmHg	Ap_Orifice inH ₂ O	Y	Standard Flow [Q _s] m ³ /min
1	0.703	754.942	22.82	22.17	58.515	1.094	1.046	0.653
2	1.001	754.951	22.99	22.44	44.435	2.340	1.530	0.944
3	1.117	754.835	23.23	22.73	38.752	2.948	1.716	1.060
4	1.170	754.975	23.31	22.88	35.376	3.257	1.804	1.116
5	1.411	755.078	23.55	23.13	24.261	4.921	2.216	1.365

Slope (a): 1.63522
Intercept (b): -0.01721
Correlation coefficient (r): 0.99975
Uncertainty (k=2): 0.015 m³/min

Table 2: The results of Q actual calibration data

Rate	Flow rate m ³ /min	Pressure [Pa] mmHg	Temperature [T _a] °C	Temperature [T _m] °C	Ap_meter mmHg	Ap_Orifice inH ₂ O	Y	Standard Flow [Q _s] m ³ /min
1	0.703	754.942	22.82	22.17	58.515	1.094	0.655	0.650
2	1.001	754.951	22.99	22.44	44.435	2.340	0.958	0.944
3	1.117	754.835	23.23	22.73	38.752	2.948	1.076	1.061
4	1.170	754.975	23.31	22.88	35.376	3.257	1.131	1.117
5	1.411	755.078	23.55	23.13	24.261	4.921	1.391	1.367

Slope (a): 1.02416
Intercept (b): -0.01068
Correlation coefficient (r): 0.99975
Uncertainty (k=2): 0.015 m³/min

End of Certificate of Calibration

Calibrated by:
Mr. Siravit Thachulad
Mr. Jiraporn Lertsomphol



Approved signature:
Mr. Parinya Booncharoen
Calibration Department Manager





THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-68/0159 MTC No. EEL. BP. 80/0168

CALIBRATION CERTIFICATE

Submitted by : Integrated Research Center Company Limited.
Address : 122 Moo 2, T.Thatoom, A.Srimahaphote, Pachinburi, 25140.
Calibrated at : Electrical and Electronic Standards Laboratory, Industrial Metrology and Testing Service Centre.
 Soi 1C, Bangpoo Industrial Estate, Sukhumvit Rd., Muang, Samutprakan 10280.

Instrument Calibrated :
 Description : Sound Calibrator
 Manufacturer : ACO
 Model : 2127
 Serial No. : 100012

Ambient Environment
 Temperature : (23 ± 3) °C
 Relative Humidity : (50 ± 15) %
 Ambient Pressure : (101.325 ± 1.500) kPa

- Standards used :**
1. Digital Function Synthesizer NF Electronic DF-193A S/N 122037.
 2. Measuring Amplifier Bruel&Kjaer 2636 S/N 1537484.
 3. Programmable Attenuator Tamagawa TPA-303A S/N OF 2214.
 4. Digital Multimeter Agilent 34401A S/N MY44005560.
 5. Pressure Transmitter Vaisala PTB202AD S/N T0650001.
 6. Audio Analyzer Panasonic VP-7722A S/N 041477D122.
 7. Condenser Microphone B&K 4180 S/N 2889871.

Calibration Procedure: CP-102-04 based on IEC 60942:2003; The sound pressure level generated by sound calibrator under test shall be measured by standard microphone using an insert voltage technique.
 This instrument has been calibrated against standards maintained at Electrical and Electronic Standards Laboratory (EEL), which are traceable to the International System of Units through the National Institute of Metrology (Thailand).

The information on actual reading is attached herewith and the uncertainty limits quoted refer to the measured values only.

Date of Receipt : 14 Jan. 2025
Date of Calibration : 21 Jan. 2025

1 / 2

The results relate only to the items tested/calibrated or value assigned.
 Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.5

Head Office
 35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
 Changwat Pathumthani 12120, Thailand
 Tel. (66) 0 2577 9036
 Fax. (66) 0 2577 9009

Office/Laboratory
 668 Mu 2 Tambon Bangpoo, Amphoe Muang Samutprakan,
 Changwat Samutprakan 10280, Thailand
 Tel. (66) 0 2323 1672-80 ext. 115, 116
 (66) 08 3219 9440
 E-mail : mtic@tistr.or.th Website : www.tistr.or.th

Office
 196 Phahonyothin Road, Ladyao, Chatuchak,
 Bangkok 10900, Thailand
 Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
 (66) 08 1889 6827



THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-68/0159 MTC No. EEL. BP. 82/0168

CALIBRATION CERTIFICATE

Submitted by : Integrated Research Center Company Limited.
Address : 122 Moo 2, T.Thatoom, A.Srimahaphote, Pachinburi, 25140.
Calibrated at : Electrical and Electronic Standards Laboratory, Industrial Metrology and Testing Service Centre.
 Soi 1C, Bangpoo Industrial Estate, Sukhumvit Rd., Muang, Samutprakan 10280.

Instrument Calibrated :
 Description : Sound Calibrator
 Manufacturer : Delta Ohm
 Model : HD9102
 Serial No. : 10038483

Ambient Environment
 Temperature : (23 ± 3) °C
 Relative Humidity : (50 ± 15) %
 Ambient Pressure : (101.325 ± 1.500) kPa

- Standards used :**
1. Digital Function Synthesizer NF Electronic DF-193A S/N 122037.
 2. Measuring Amplifier Bruel&Kjaer 2636 S/N 1537484.
 3. Programmable Attenuator Tamagawa TPA-303A S/N OF 2214.
 4. Digital Multimeter Agilent 34401A S/N MY44005560.
 5. Pressure Transmitter Vaisala PTB202AD S/N T0650001.
 6. Audio Analyzer Panasonic VP-7722A S/N 041477D122.
 7. Condenser Microphone B&K 4180 S/N 2889871.

Calibration Procedure: CP-102-04 based on IEC 60942:2003. The sound pressure level of instrument was measured by standard microphone using an insert voltage technique.

This instrument has been calibrated against standards maintained at Electrical and Electronic Standards Laboratory (EEL), which are traceable to the International System of Units through the National Institute of Metrology (Thailand).

The information on actual reading is attached herewith and the uncertainty limits quoted refer to the measured values only.

Date of Receipt : 14 Jan. 2025
Date of Calibration : 22 Jan. 2025

1 / 3

The results relate only to the items tested/calibrated or value assigned.
 Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.5

Head Office
 35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
 Changwat Pathumthani 12120, Thailand
 Tel. (66) 0 2577 9036
 Fax. (66) 0 2577 9009

Office/Laboratory
 668 Mu 2 Tambon Bangpoo, Amphoe Muang Samutprakan,
 Changwat Samutprakan 10280, Thailand
 Tel. (66) 0 2323 1672-80 ext. 115, 116
 (66) 08 3219 9440
 E-mail : mtic@tistr.or.th Website : www.tistr.or.th

Office
 196 Phahonyothin Road, Ladyao, Chatuchak,
 Bangkok 10900, Thailand
 Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
 (66) 08 1889 6827



THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-68/0159 MTC No. EEL. BP. 80/0168

The reported expanded uncertainty is based upon a standard uncertainty multiplied by a coverage factor k = 2, providing a level of confidence of approximately 95%.

Nominal Output of Unit Under Test = 94 dB re 20µPa at 1000 Hz

Acoustic Output in dB re 20µPa, Corrected to Reference Conditions : 101.325 kPa, 23.0 °C and 50 %RH.

1. Sound Pressure Level

Standard Microphone Type	Measured Sound Pressure Level (dB)	Deviated value (dB)	Uncertainty (dB)	Tolerance limit IEC60942:2003 Class 1
1/2 inch Bruel&Kjaer 4180	93.91	-0.09	± 0.10	±0.40 dB

2. Frequency

Standard Microphone Type	Measured Frequency (Hz)	Deviated value (Hz)	Uncertainty (Hz)	Tolerance limit IEC60942:2003 Class 1
1/2 inch Bruel&Kjaer 4180	1000.0	0.0	± 1.5	±1.0%

3. Total Distortion

Standard Microphone Type	Measured Total Distortion (%)	Uncertainty (%)	Tolerance limit IEC60942:2003 Class 1
1/2 inch Bruel&Kjaer 4180	1.50	± 0.50	±3.0%

- Note :**
1. No adjustment.
 2. The calibrator pressure correction was not included.
 3. The microphone volume correction was not included.

Calibrated by :
 (Mr.Weerchai Deechaiyae)

Approved by :
 Director
 Electrical and Electronic Standards Laboratory
 Industrial Metrology and Testing Service Centre

Date of Calibration : 21 Jan. 2025
Date of Issue : 23 Jan. 2025

Ref : 2011268011400184001

End of Certificate

2 / 2

The results relate only to the items tested/calibrated or value assigned.
 Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.5

Head Office
 35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
 Changwat Pathumthani 12120, Thailand
 Tel. (66) 0 2577 9036
 Fax. (66) 0 2577 9009

Office/Laboratory
 668 Mu 2 Tambon Bangpoo, Amphoe Muang Samutprakan,
 Changwat Samutprakan 10280, Thailand
 Tel. (66) 0 2323 1672-80 ext. 115, 116
 (66) 08 3219 9440
 E-mail : mtic@tistr.or.th Website : www.tistr.or.th

Office
 196 Phahonyothin Road, Ladyao, Chatuchak,
 Bangkok 10900, Thailand
 Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
 (66) 08 1889 6827



THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-68/0159 MTC No. EEL. BP. 82/0168

The reported expanded uncertainty is based upon a standard uncertainty multiplied by a coverage factor k = 2, providing a level of confidence of approximately 95%.

Nominal Output of Unit Under Test = 94 dB re 20µPa at 1000 Hz

Acoustic Output in dB re 20µPa, Corrected to Reference Conditions : 101.325 kPa, 23.0°C and 50 %RH

1. Sound Pressure Level

Standard Microphone Type	Measured Sound Pressure Level (dB)	Deviated value (dB)	Uncertainty (dB)	Tolerance limit IEC60942:2003 Class 2
1/2 inch Bruel&Kjaer 4180	93.88	-0.12	± 0.10	±0.75 dB

2. Frequency

Standard Microphone Type	Measured Frequency (Hz)	Deviated value (Hz)	Uncertainty (Hz)	Tolerance limit IEC60942:2003 Class 2
1/2 inch Bruel&Kjaer 4180	988.3	-11.7	± 1.5	±2.0%

3. Total distortion

Standard Microphone Type	Measured Total distortion (%)	Uncertainty (%)	Tolerance limit IEC60942:2003 Class 2
1/2 inch Bruel&Kjaer 4180	1.00	± 0.50	±4.0%

- Note :**
1. No adjustment.
 2. The calibrator pressure correction was not included.
 3. The microphone volume correction was not included.

Date of Calibration : 22 Jan. 2025

2 / 3

The results relate only to the items tested/calibrated or value assigned.
 Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.5

Head Office
 35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
 Changwat Pathumthani 12120, Thailand
 Tel. (66) 0 2577 9036
 Fax. (66) 0 2577 9009

Office/Laboratory
 668 Mu 2 Tambon Bangpoo, Amphoe Muang Samutprakan,
 Changwat Samutprakan 10280, Thailand
 Tel. (66) 0 2323 1672-80 ext. 115, 116
 (66) 08 3219 9440
 E-mail : mtic@tistr.or.th Website : www.tistr.or.th

Office
 196 Phahonyothin Road, Ladyao, Chatuchak,
 Bangkok 10900, Thailand
 Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
 (66) 08 1889 6827



THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-68/0159

MTC No. EEL. BP. 82/0168

Nominal Output of Unit Under Test = 114 dB re 20µPa at 1000 Hz

Acoustic Output in dB re 20µPa, Corrected to Reference Conditions: 101.325 kPa, 23.0 °C and 50 %RH

1. Sound Pressure Level

Table with 5 columns: Standard Microphone Type, Measured Sound Pressure Level (dB), Deviated value (dB), Uncertainty (dB), Tolerance limit (IEC60942:2003 Class 2). Row 1: 1/2 inch Bruel&Kjaer 4180, 113.86, -0.14, ± 0.10, ±0.75 dB

2. Frequency

Table with 5 columns: Standard Microphone Type, Measured Frequency (Hz), Deviated value (Hz), Uncertainty (Hz), Tolerance limit (IEC60942:2003 Class 2). Row 1: 1/2 inch Bruel&Kjaer 4180, 988.4, -11.6, ± 1.5, ±2.0%

3. Total Distortion

Table with 4 columns: Standard Microphone Type, Measured Total Distortion (%), Uncertainty (%), Tolerance limit (IEC60942:2003 Class 2). Row 1: 1/2 inch Bruel&Kjaer 4180, 0.21, ± 0.50, ±4.0%

Note: 1. No adjustment.

2. The calibrator pressure correction was not included.

3. The microphone volume correction was not included.

Calibrated by: (Mr. Weerachai Deechaiyai)

Approved by: (Mr. Prasit Kiatyapa)



Electrical and Electronic Standards Laboratory

Industrial Metrology and Testing Service Centre

Date of Calibration: 22 Jan. 2025

Date of Issue: 23 Jan. 2025

Ref: 2011268011400184003

End of Certificate

3 / 3

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FMBL/MTC.002 Rev.5



THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-68/0159

MTC No. EEL. BP. 81/0168

CALIBRATION CERTIFICATE

Submitted by: Integrated Research Center Company Limited.

Address: 122 Moo 2, T. Thatoom, A.Srimahaphote, Prachinburi, 25140.

Calibrated at: Electrical and Electronic Standards Laboratory, Industrial Metrology and Testing Service Centre.

Soi 1C, Bangpoo Industrial Estate, Sukhumvit Rd., Muang, Samutprakarn 10280.

Instrument Calibrated:

Description: Sound Calibrator

Manufacturer: Rion

Model: NC-74

Serial No.: 35046798

Ambient Environment

Temperature: (23 ± 3) °C

Relative Humidity: (50 ± 15) %

Ambient Pressure: (101.325 ± 1.500) kPa

Standards used: 1. Digital Function Synthesizer NF Electronic DF-193A S/N 122037.

2. Measuring Amplifier Bruel&Kjaer 2636 S/N 1537484.

3. Programmable Attenuator Tamagawa TPA-303A S/N OF 2214.

4. Digital Multimeter Agilent 34401A S/N MY44005560.

5. Pressure Transmitter Vaisala PTB202AD S/N T0650001.

6. Audio Analyzer Panasonic VP-7722A S/N 041477D122.

7. Condenser Microphone B&K 4180 S/N 2633526.

Calibration Procedure: CP-102-04 based on IEC 60942:2003; The sound pressure level generated by sound calibrator under test shall be measured by standard microphone using an insert voltage technique.

This instrument has been calibrated against standards maintained at Electrical and Electronic Standards Laboratory (EEL), which are traceable to the International System of Units through the National Institute of Metrology (Thailand).

The information on actual reading is attached herewith and the uncertainty limits quoted refer to the measured values only.

The information on actual reading is attached herewith and the uncertainty limits quoted refer to the measured values only.

The information on actual reading is attached herewith and the uncertainty limits quoted refer to the measured values only.

The information on actual reading is attached herewith and the uncertainty limits quoted refer to the measured values only.

The information on actual reading is attached herewith and the uncertainty limits quoted refer to the measured values only.

Date of Receipt: 14 Jan. 2025

Date of Calibration: 22 Jan. 2025

1 / 2

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FMBL/MTC.002 Rev.5



THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-68/0159

MTC No. EEL. BP. 81/0168

The reported expanded uncertainty is based upon a standard uncertainty multiplied by a coverage factor k = 2, providing a level of confidence of approximately 95%.

The reported expanded uncertainty is based upon a standard uncertainty multiplied by a coverage factor k = 2, providing a level of confidence of approximately 95%.

Nominal Output of Unit Under Test = 94 dB re 20µPa at 1000 Hz

Acoustic Output in dB re 20µPa, Corrected to Reference Conditions: 101.325 kPa, 23.0 °C and 50 %RH.

1. Sound Pressure Level

Table with 5 columns: Standard Microphone Type, Measured Sound Pressure Level (dB), Deviated value (dB), Uncertainty (dB), Tolerance limit (IEC60942:2003 Class 1). Row 1: 1/2 inch Bruel&Kjaer 4180, 93.91, -0.09, ± 0.10, ±0.40 dB

2. Frequency

Table with 5 columns: Standard Microphone Type, Measured Frequency (Hz), Deviated value (Hz), Uncertainty (Hz), Tolerance limit (IEC60942:2003 Class 1). Row 1: 1/2 inch Bruel&Kjaer 4180, 1001.5, 1.5, ± 1.5, ±1.0%

3. Total Distortion

Table with 4 columns: Standard Microphone Type, Measured Total Distortion (%), Uncertainty (%), Tolerance limit (IEC60942:2003 Class 1). Row 1: 1/2 inch Bruel&Kjaer 4180, 1.35, ± 0.50, ±3.0%

Note: 1. No adjustment.

2. The calibrator pressure correction was not included.

3. The microphone volume correction was included at level of 0.16 dB from manual.

Calibrated by: (Mr. Weerachai Deechaiyai)

Approved by: (Mr. Prasit Kiatyapa)



Electrical and Electronic Standards Laboratory

Industrial Metrology and Testing Service Centre

Date of Calibration: 22 Jan. 2025

Date of Issue: 23 Jan. 2025

Ref: 2011268011400184002

End of Certificate

2 / 2

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FMBL/MTC.002 Rev.5



THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-68/0160

MTC No. EEL. BP. 89/0168

CALIBRATION CERTIFICATE

Submitted by: Integrated Research Center Company Limited.

Address: 122 Moo 2, T. Thatoom, A.Srimahaphote, Prachinburi, 25140.

Calibrated at: Electrical and Electronic Standards Laboratory, Industrial Metrology and Testing Service Centre.

Soi 1C, Bangpoo Industrial Estate, Sukhumvit Rd., A.Muang, Samutprakarn 10280.

Instrument Calibrated:

Description: Integrating Sound Level Meter

Manufacturer: ACO

Model: 6226

Serial No.: 100144

Microphone: Type 7052 No.79844

Preamplifier: -

Ambient Environment

Temperature: (23 ± 3) °C

Relative Humidity: (50 ± 15) %

Ambient Pressure: (101.325±1.5) kPa

Standards used: 1. Band Pass Filter Stanford Research Systems SR 650 S/N 28712.

2. Condenser Microphone Bruel&Kjaer 4180 S/N 2889871.

3. Decade Attenuator Ando AL-205 S/N 00464602.

4. Function/Arbitrary Waveform Generator Agilent 33220A S/N MY44042668.

5. Digital Function Synthesizer NF Electronic Instruments DF-193A S/N 122037.

6. Sound Calibrator Bruel&Kjaer 4231 S/N 3015154.

7. Measuring Amplifier Bruel&Kjaer 2636 S/N 1537484.

Date of Receipt: 14 Jan. 2025

Date of Calibration: 17-18 Feb. 2025

1 / 9

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FMBL/MTC.002 Rev.5



Head Office: 35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang, Changwat Pathumthani 12120, Thailand. Tel. (66) 0 2577 9036. Fax. (66) 0 2577 9009.

Office/Laboratory: 668 Mu 2 Tambon Bangpoomai, Amphoe Muang Samutprakarn, Changwat Samutprakarn 10280, Thailand. Tel. (66) 0 2323 1672-80 ext. 115, 116. (66) 08 3219 9440. E-mail: mtg@tistr.or.th Website: www.tistr.or.th

Office: 196 Phahonyothin Road, Ladyao, Chatuchak, Bangkok 10900, Thailand. Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217. (66) 08 1889 6827

Head Office: 35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang, Changwat Pathumthani 12120, Thailand. Tel. (66) 0 2577 9036. Fax. (66) 0 2577 9009.

Office/Laboratory: 668 Mu 2 Tambon Bangpoomai, Amphoe Muang Samutprakarn, Changwat Samutprakarn 10280, Thailand. Tel. (66) 0 2323 1672-80 ext. 115, 116. (66) 08 3219 9440. E-mail: mtg@tistr.or.th Website: www.tistr.or.th

Office: 196 Phahonyothin Road, Ladyao, Chatuchak, Bangkok 10900, Thailand. Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217. (66) 08 1889 6827

8. Power Amplifier Brüel&Kjær 2706 S/N 1517650.
9. Speaker Tannoy Limited, Great Britain British Patent No. 215300.
10. Digital Multimeter Agilent 34401A S/N MY44005560.
11. Programmable Attenuator Tamagawa TPA-303A S/N 2212.

Calibration Procedure :

This instrument was calibrated by using calibration procedures no CP-102-02 and CP-102-03, which were based on IEC 61672-3 Electroacoustics - Sound Level Meters - Part 3 : Periodic tests (2013). These calibration procedures were related to the electrical and acoustic signal tests. The electrical signal test was carried out with the direct measurement method. The acoustic signal test was performed in an anechoic room with the comparison measurement method.

This instrument has been calibrated against standards maintained at the Electrical and Electronic Standards Laboratory (EEL), which are traceable to the International System of Units through the National Institute of Metrology (Thailand).

The information on actual reading is attached herewith and the uncertainty limits quoted refer to the measured values only.

The reported expanded uncertainty is based upon a standard uncertainty multiplied by a coverage factor $k=2$, providing a level of confidence of approximately 95%.

Date of Calibration : 17-18 Feb. 2025

2 / 9

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BLMTC.002 Rev.5

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9059

Office/Laboratory
668 Mu 2 Tambon Bangpoornai, Amphoe Muang Samutprakan,
Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtg@tistr.or.th Website : www.tistr.or.th

Office
196 Phahonyothin Road, Ladysao, Chatuchak,
Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827

3. Acoustical signal test of frequency weightings

Frequency (Hz)	Deviation from frequency response (dB)			Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
	A-weight	C-weight	Flat			
125	-0.3	0.2	0.1	1.5	0.45	0.6
1 000	-0.1	-0.1	0.0	1.0	0.45	0.6
8 000	-4.8	-4.7	-4.8	5.0	0.45	0.7

4. Electrical signal test of frequency weightings

Frequency (Hz)	Deviation from frequency response (dB)			Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
	A-weight	C-weight	Flat			
63	0.2	0.1	0.1	2.0	0.20	0.6
125	0.1	0.2	0.1	1.5	0.20	0.6
250	0.2	0.1	0.1	1.5	0.20	0.6
500	0.1	0.0	0.0	1.5	0.20	0.6
1 000	0.0	0.0	0.0	1.0	0.20	0.6
2 000	-0.1	0.0	0.1	2.0	0.20	0.6
4 000	-0.4	-0.2	0.0	3.0	0.20	0.6
8 000	-0.4	-0.2	-0.1	5.0	0.20	0.7

Date of Calibration : 17-18 Feb. 2025

4 / 9

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BLMTC.002 Rev.5

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9059

Office/Laboratory
668 Mu 2 Tambon Bangpoornai, Amphoe Muang Samutprakan,
Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtg@tistr.or.th Website : www.tistr.or.th

Office
196 Phahonyothin Road, Ladysao, Chatuchak,
Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827

1. Absolute Sensitivity

Reference Acoustic Signal (dB)	Measured value (dB)		Deviation value (dB)	Acceptance limit Class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
	Before adjust	After adjust				
93.99	93.7	94.0	0.0	1.0	0.30	N/A

Note: The external calibration adjustment was firstly performed. The internal calibration adjustment was then completed at the display of 115.1 dB.

2. Self-generated noise

2.1 Normal test

Measured value (dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
18.5	0.10	N/A

2.2 The microphone of the sound level meter was replaced by electrical signal input device

Frequency Weighting	Measured value (dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
A-Weight	16.3	0.10	N/A
C-Weight	24.7	0.10	N/A
Flat	26.7	0.10	N/A

Date of Calibration : 17-18 Feb. 2025

3 / 9

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BLMTC.002 Rev.5

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9059

Office/Laboratory
668 Mu 2 Tambon Bangpoornai, Amphoe Muang Samutprakan,
Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtg@tistr.or.th Website : www.tistr.or.th

Office
196 Phahonyothin Road, Ladysao, Chatuchak,
Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827

5. Long-term stability

Time	Measured Value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Begin	94.0	0.0	0.3	0.10	0.1
End	94.0				

6. Frequency and time weightings at 1 kHz

6.1 Frequency weightings at 1 kHz

Frequency Weighting	Measured Value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
A-weight	94.0	0.0	0.2	0.20	0.2
C-weight	94.0	0.0	0.2	0.20	0.2
Flat	94.1	0.1	0.2	0.20	0.2

6.2 Time weightings at 1 kHz

Frequency Weighting	Measured Value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Fast	94.0	0.0	0.1	0.20	0.2
Slow	94.0	0.0	0.1	0.20	0.2
Leq	94.0	0.0	0.1	0.20	0.2

Date of Calibration : 17-18 Feb. 2025

5 / 9

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BLMTC.002 Rev.5

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9059

Office/Laboratory
668 Mu 2 Tambon Bangpoornai, Amphoe Muang Samutprakan,
Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtg@tistr.or.th Website : www.tistr.or.th

Office
196 Phahonyothin Road, Ladysao, Chatuchak,
Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827

7. Level linearity on the reference level range

Anticipated value (dB)	Measured Value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
122	122.0	0.0	1.1	0.30	0.3
121	121.1	0.1	1.1	0.30	0.3
120	120.0	0.0	1.1	0.30	0.3
119	119.1	0.1	1.1	0.30	0.3
114	114.0	0.0	1.1	0.30	0.3
109	109.0	0.0	1.1	0.30	0.3
104	104.0	0.0	1.1	0.30	0.3
99	99.1	0.1	1.1	0.30	0.3
94	94.0	0.0	1.1	0.30	0.3
89	89.0	0.0	1.1	0.30	0.3
84	84.1	0.1	1.1	0.30	0.3
79	79.1	0.1	1.1	0.30	0.3
74	74.1	0.1	1.1	0.30	0.3
69	69.1	0.1	1.1	0.30	0.3
64	64.0	0.0	1.1	0.30	0.3
59	59.0	0.0	1.1	0.30	0.3
54	54.0	0.0	1.1	0.30	0.3
49	49.0	0.0	1.1	0.30	0.3
44	44.1	0.1	1.1	0.30	0.3
39	39.0	0.0	1.1	0.30	0.3
34	34.1	0.1	1.1	0.30	0.3
33	33.1	0.1	1.1	0.30	0.3

Date of Calibration : 17-18 Feb. 2025

6/9

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full, are prohibited unless written permission is obtained from the governor of TISTR.

FMBL/MTC.002 Rev.5

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang, Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9009

Office/Laboratory
668 Mu 2 Tambon Bangpoomai, Amphoe Muang Samutprakarn, Changwat Samutprakarn 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtic@tistr.or.th Website : www.tistr.or.th

Office
196 Phahonyothin Road, Ladysao, Chatuchak, Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5231
(66) 08 1889 6827

8. Level linearity including the level range control

At reference level at 5 dB greater than the under-range on a level range

Range	Anticipated value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
40-130	45	45.0	0.0	1.1	0.30	0.3
30-120	35	35.0	0.0	1.1	0.30	0.3
20-110	25	25.5	0.5	1.1	0.30	0.3
20-100	25	25.5	0.5	1.1	0.30	0.3
20-90	25	25.4	0.4	1.1	0.30	0.3
20-80	25	25.4	0.4	1.1	0.30	0.3

9. Tone burst response

Time Weighting	Toneburst Duration, Tb (ms)	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Fast	200	115.8	-0.2	±1.0	0.20	0.3
	2	98.8	-0.2	+1.0; -2.5	0.20	0.3
	0.25	89.6	-0.4	+1.5; -5.0	0.20	0.3
Slow	200	109.4	-0.2	±1.0	0.20	0.3
	2	89.8	-0.2	+1.0; -5.0	0.20	0.3
SEL	200	109.9	-0.1	±1.0	0.20	0.3
	2	90.0	0.0	+1.0; -2.5	0.20	0.3
	0.25	80.9	-0.1	+1.5; -5.0	0.20	0.3

Date of Calibration : 17-18 Feb. 2025

8/9

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full, are prohibited unless written permission is obtained from the governor of TISTR.

FMBL/MTC.002 Rev.5

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang, Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9009

Office/Laboratory
668 Mu 2 Tambon Bangpoomai, Amphoe Muang Samutprakarn, Changwat Samutprakarn 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtic@tistr.or.th Website : www.tistr.or.th

Office
196 Phahonyothin Road, Ladysao, Chatuchak, Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5231
(66) 08 1889 6827

7. Level linearity on the reference level range

Anticipated value (dB)	Measured Value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
32	32.1	0.1	1.1	0.30	0.3
31	31.3	0.3	1.1	0.30	0.3
30	30.3	0.3	1.1	0.30	0.3

8. Level linearity including the level range control

At reference sound level on the reference level range

Range	Anticipated value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
40-130	94.0	94.0	0.0	1.1	0.30	0.3
30-120	94.0	94.0	0.0	1.1	0.30	0.3
20-110	94.0	94.0	0.0	1.1	0.30	0.3
20-100	94.0	94.0	0.0	1.1	0.30	0.3

Date of Calibration : 17-18 Feb. 2025

7/9

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full, are prohibited unless written permission is obtained from the governor of TISTR.

FMBL/MTC.002 Rev.5

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang, Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9009

Office/Laboratory
668 Mu 2 Tambon Bangpoomai, Amphoe Muang Samutprakarn, Changwat Samutprakarn 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtic@tistr.or.th Website : www.tistr.or.th

Office
196 Phahonyothin Road, Ladysao, Chatuchak, Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5231
(66) 08 1889 6827

10. Peak C sound level

Number of cycles in test signal	Anticipated value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Complete cycle	125.4	125.8	0.4	3.0	0.20	0.35
Positive half cycle	124.4	124.2	-0.2	2.0	0.20	0.35
Negative half cycle	124.4	124.2	-0.2	2.0	0.20	0.35

11. Overload indication

Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)		
Positive one-half cycle	Negative one-half cycle	131.1	0.0	1.5	0.20	0.25

12. High-level stability

Time	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Begin	129.0	0.0	0.3	0.10	0.1
End	129.0				

Calibrated by:
(Mr. Pannasit Phasingari)

Approved by:
(Mr. Pravithe Khuyyap)
Director

Date of Calibration : 17-18 Feb. 2025

Date of Issue : 24 Feb. 2025

Electrical and Electronic Standards Laboratory

Industrial Metrology and Testing Service Centre

Ref : 2011268011400185007

End of Certificate

9/9

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full, are prohibited unless written permission is obtained from the governor of TISTR.

FMBL/MTC.002 Rev.5

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang, Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9009

Office/Laboratory
668 Mu 2 Tambon Bangpoomai, Amphoe Muang Samutprakarn, Changwat Samutprakarn 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtic@tistr.or.th Website : www.tistr.or.th

Office
196 Phahonyothin Road, Ladysao, Chatuchak, Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5231
(66) 08 1889 6827



CALIBRATION CERTIFICATE

Submitted by : Integrated Research Center Company Limited.

Address : 122 Moo 2, T.Thatoom, A.Srimahaphote, Prachinburi, 25140.

Calibrated at : Electrical and Electronic Standards Laboratory, Industrial Metrology and Testing Service Centre.
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Rd., A.Muang, Samutprakan 10280.

Instrument Calibrated :

Description : Integrating Sound Level Meter

Manufacturer : ACO

Model : 6226

Serial No. : 100145

Microphone : Type 7052NR No.78402

Preamplifier : -

Ambient Environment

Temperature : (23 ± 3) °C

Relative Humidity : (50 ± 15) %

Ambient Pressure : (101.325 ± 1.5) kPa

Standards used :

1. Band Pass Filter Stanford Research Systems SR 650 S/N 28712.
2. Condenser Microphone Brüel&Kjær 4180 S/N 2889871.
3. Decade Attenuator Ando AL-205 S/N 00464602.
4. Function/Arbitrary Waveform Generator Agilent 33220A S/N MY44042668.
5. Digital Function Synthesizer NF Electronic Instruments DF-193A S/N 122037.
6. Sound Calibrator Bruel&Kjaer 4231 S/N 3015154.
7. Measuring Amplifier Brüel&Kjær 2636 S/N 1537484.

Date of Receipt : 14 Jan. 2025

Date of Calibration : 17-18 Feb. 2025

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

1 / 9

FM.BLMTC.002 Rev.5

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9009Office/Laboratory
668 Mu 2 Tambon Bangpooai, Amphoe Muang Samutprakan,
Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtc@tistr.or.th Website : www.tistr.or.thOffice
196 Phahonyothin Road, Ladysa, Chatuchak,
Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827

1. Absolute Sensitivity

Reference Acoustic Signal (dB)	Measured value (dB)		Deviation value (dB)	Acceptance limit Class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
	Before adjust	After adjust				
93.99	92.9	94.0	0.0	1.0	0.30	N/A

Note: The external calibration adjustment was firstly performed. The internal calibration adjustment was then completed at the display of 117.0 dB.

2. Self-generated noise

2.1 Normal test

Measured value (dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
25.3	0.10	N/A

2.2 The microphone of the sound level meter was replaced by electrical signal input device

Frequency Weighting	Measured value (dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
A-Weight	24.5	0.10	N/A
C-Weight	26.7	0.10	N/A
Flat	31.3	0.10	N/A

Date of Calibration : 17-18 Feb. 2025

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

3 / 9

FM.BLMTC.002 Rev.5

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9009Office/Laboratory
668 Mu 2 Tambon Bangpooai, Amphoe Muang Samutprakan,
Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtc@tistr.or.th Website : www.tistr.or.thOffice
196 Phahonyothin Road, Ladysa, Chatuchak,
Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827

8. Power Amplifier Brüel&Kjær 2706 S/N 1517650.
9. Speaker Tannoy Limited, Great Britain British Patent No. 215300.
10. Digital Multimeter Agilent 34401A S/N MY44005560.
11. Programmable Attenuator Tamagawa TPA-303A S/N 2212.

Calibration Procedure :

This instrument was calibrated by using calibration procedures no CP-102-02 and CP-102-03, which were based on IEC 61672-3 Electroacoustics - Sound Level Meters - Part 3 : Periodic tests (2013). These calibration procedures were related to the electrical and acoustic signal tests. The electrical signal test was carried out with the direct measurement method. The acoustic signal test was performed in an anechoic room with the comparison measurement method.

This instrument has been calibrated against standards maintained at the Electrical and Electronic Standards Laboratory (EEL), which are traceable to the International System of Units through the National Institute of Metrology (Thailand).

The information on actual reading is attached herewith and the uncertainty limits quoted refer to the measured values only.

The reported expanded uncertainty is based upon a standard uncertainty multiplied by a coverage factor $k=2$, providing a level of confidence of approximately 95%.

Date of Calibration : 17-18 Feb. 2025

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

2 / 9

FM.BLMTC.002 Rev.5

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9009Office/Laboratory
668 Mu 2 Tambon Bangpooai, Amphoe Muang Samutprakan,
Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtc@tistr.or.th Website : www.tistr.or.thOffice
196 Phahonyothin Road, Ladysa, Chatuchak,
Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827

3. Acoustical signal test of frequency weightings

Frequency (Hz)	Deviation from frequency response (dB)			Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
	A-weight	C-weight	Flat			
125	0.4	0.1	-0.1	1.5	0.45	0.6
1 000	0.1	0.2	0.2	1.0	0.45	0.6
8 000	-4.2	-3.6	-4.4	5.0	0.45	0.7

4. Electrical signal test of frequency weightings

Frequency (Hz)	Deviation from frequency response (dB)			Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
	A-weight	C-weight	Flat			
63	0.1	0.1	0.1	2.0	0.20	0.6
125	0.1	0.1	0.1	1.5	0.20	0.6
250	0.1	0.1	0.1	1.5	0.20	0.6
500	0.1	0.0	0.0	1.5	0.20	0.6
1 000	0.0	0.0	0.0	1.0	0.20	0.6
2 000	-0.1	0.0	0.1	2.0	0.20	0.6
4 000	-0.3	-0.1	0.0	3.0	0.20	0.6
8 000	-0.3	-0.1	-0.1	5.0	0.20	0.7

Date of Calibration : 17-18 Feb. 2025

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

4 / 9

FM.BLMTC.002 Rev.5

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9009Office/Laboratory
668 Mu 2 Tambon Bangpooai, Amphoe Muang Samutprakan,
Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtc@tistr.or.th Website : www.tistr.or.thOffice
196 Phahonyothin Road, Ladysa, Chatuchak,
Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827

5. Long-term stability

Time	Measured Value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Begin	94.0	0.0	0.3	0.10	0.1
End	94.0				

6. Frequency and time weightings at 1 kHz
6.1 Frequency weightings at 1 kHz

Frequency Weighting	Measured Value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
A-weight	94.0	0.0	0.2	0.20	0.2
C-weight	94.0	0.0	0.2	0.20	0.2
Flat	94.1	0.1	0.2	0.20	0.2

6.2 Time weightings at 1 kHz

Frequency Weighting	Measured Value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Fast	94.0	0.0	0.1	0.20	0.2
Slow	94.0	0.0	0.1	0.20	0.2
Leq	94.0	0.0	0.1	0.20	0.2

Date of Calibration : 17-18 Feb. 2025

5 / 9

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FMLB/MTC.002 Rev.5

Head Office
 35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
 Changwat Pathumthani 12120, Thailand
 Tel. (66) 0 2577 9036
 Fax. (66) 0 2577 9009

Office/Laboratory
 668 Mu 2 Tambon Bangpoomai, Amphoe Muang Samutprakan,
 Changwat Samutprakan 10280, Thailand
 Tel. (66) 0 2323 1672-80 ext. 115, 116
 (66) 08 3219 9440
 E-mail : mtic@tistr.or.th Website : www.tistr.or.th

Office
 196 Phahonyothin Road, Ladysao, Chatuchak,
 Bangkok 10900, Thailand
 Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5237
 (66) 08 1889 6827

7. Level linearity on the reference level range

Anticipated value (dB)	Measured Value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
32	32.2	0.2	1.1	0.30	0.3
31	31.2	0.2	1.1	0.30	0.3
30	30.3	0.3	1.1	0.30	0.3

8. Level linearity including the level range control

At reference sound level on the reference level range

Range (dB)	Anticipated value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
40-130	94.0	94.0	0.0	1.1	0.30	0.3
30-120	94.0	94.0	0.0	1.1	0.30	0.3
20-110	94.0	94.0	0.0	1.1	0.30	0.3
20-100	94.0	94.0	0.0	1.1	0.30	0.3

Date of Calibration : 17-18 Feb. 2025

7 / 9

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FMLB/MTC.002 Rev.5

Head Office
 35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
 Changwat Pathumthani 12120, Thailand
 Tel. (66) 0 2577 9036
 Fax. (66) 0 2577 9009

Office/Laboratory
 668 Mu 2 Tambon Bangpoomai, Amphoe Muang Samutprakan,
 Changwat Samutprakan 10280, Thailand
 Tel. (66) 0 2323 1672-80 ext. 115, 116
 (66) 08 3219 9440
 E-mail : mtic@tistr.or.th Website : www.tistr.or.th

Office
 196 Phahonyothin Road, Ladysao, Chatuchak,
 Bangkok 10900, Thailand
 Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5237
 (66) 08 1889 6827

7. Level linearity on the reference level range

Anticipated value (dB)	Measured Value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
122	121.9	-0.1	1.1	0.30	0.3
121	120.9	-0.1	1.1	0.30	0.3
120	119.9	-0.1	1.1	0.30	0.3
119	119.0	0.0	1.1	0.30	0.3
114	113.9	-0.1	1.1	0.30	0.3
109	108.9	-0.1	1.1	0.30	0.3
104	103.9	-0.1	1.1	0.30	0.3
99	99.0	0.0	1.1	0.30	0.3
94	94.0	0.0	1.1	0.30	0.3
89	88.9	-0.1	1.1	0.30	0.3
84	84.0	0.0	1.1	0.30	0.3
79	79.0	0.0	1.1	0.30	0.3
74	74.0	0.0	1.1	0.30	0.3
69	69.0	0.0	1.1	0.30	0.3
64	63.9	-0.1	1.1	0.30	0.3
59	58.9	-0.1	1.1	0.30	0.3
54	53.9	-0.1	1.1	0.30	0.3
49	48.9	-0.1	1.1	0.30	0.3
44	44.0	0.0	1.1	0.30	0.3
39	38.9	-0.1	1.1	0.30	0.3
34	34.0	0.0	1.1	0.30	0.3
33	33.1	0.1	1.1	0.30	0.3

Date of Calibration : 17-18 Feb. 2025

6 / 9

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FMLB/MTC.002 Rev.5

Head Office
 35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
 Changwat Pathumthani 12120, Thailand
 Tel. (66) 0 2577 9036
 Fax. (66) 0 2577 9009

Office/Laboratory
 668 Mu 2 Tambon Bangpoomai, Amphoe Muang Samutprakan,
 Changwat Samutprakan 10280, Thailand
 Tel. (66) 0 2323 1672-80 ext. 115, 116
 (66) 08 3219 9440
 E-mail : mtic@tistr.or.th Website : www.tistr.or.th

Office
 196 Phahonyothin Road, Ladysao, Chatuchak,
 Bangkok 10900, Thailand
 Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5237
 (66) 08 1889 6827

8. Level linearity including the level range control

At reference level at 5 dB greater than the under-range on a level range

Range (dB)	Anticipated value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
40-130	45	45.0	0.0	1.1	0.30	0.3
30-120	35	35.0	0.0	1.1	0.30	0.3
20-110	25	25.4	0.4	1.1	0.30	0.3
20-100	25	25.5	0.5	1.1	0.30	0.3
20-90	25	25.6	0.6	1.1	0.30	0.3
20-80	25	25.5	0.5	1.1	0.30	0.3

9. Tone burst response

Time Weighting	Toneburst Duration, Tb (ms)	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Fast	200	115.8	-0.2	±1.0	0.20	0.3
	2	98.8	-0.2	+1.0; -2.5	0.20	0.3
	0.25	89.6	-0.4	+1.5; -5.0	0.20	0.3
Slow	200	109.4	-0.2	±1.0	0.20	0.3
	2	89.8	-0.2	+1.0; -5.0	0.20	0.3
SEL	200	109.9	-0.1	±1.0	0.20	0.3
	2	90.0	0.0	+1.0; -2.5	0.20	0.3
	0.25	80.9	-0.1	+1.5; -5.0	0.20	0.3

Date of Calibration : 17-18 Feb. 2025

8 / 9

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FMLB/MTC.002 Rev.5

Head Office
 35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
 Changwat Pathumthani 12120, Thailand
 Tel. (66) 0 2577 9036
 Fax. (66) 0 2577 9009

Office/Laboratory
 668 Mu 2 Tambon Bangpoomai, Amphoe Muang Samutprakan,
 Changwat Samutprakan 10280, Thailand
 Tel. (66) 0 2323 1672-80 ext. 115, 116
 (66) 08 3219 9440
 E-mail : mtic@tistr.or.th Website : www.tistr.or.th

Office
 196 Phahonyothin Road, Ladysao, Chatuchak,
 Bangkok 10900, Thailand
 Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5237
 (66) 08 1889 6827

10. Peak C sound level

Number of cycles in test signal	Anticipated value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Complete cycle	125.4	125.8	0.4	3.0	0.20	0.35
Positive half cycle	124.4	124.2	-0.2	2.0	0.20	0.35
Negative half cycle	124.4	124.2	-0.2	2.0	0.20	0.35

11. Overload indication

Measured value (dB)		Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Positive one-half cycle	Negative one-half cycle				
131.1	131.1	0.0	1.5	0.20	0.25

12. High-level stability

Time	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Begin	129.0	0.0	0.3	0.10	0.1
End	129.0				

Calibrated by
(Mr. Pannasit Phasingsri)

Approved by:
(Mr. Pravit Kijyapa)
Director
Electrical and Electronic Standards Laboratory
Industrial Metrology and Testing Service Centre

Date of Calibration : 17-18 Feb. 2025
Date of Issue : 24 Feb. 2025

Ref: 2011268011400185008

End of Certificate

9 / 9

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BLMTC.002 Rev.5

CALIBRATION CERTIFICATE

Submitted by : Integrated Research Center Company Limited.

Address : 122 Moo 2, T.Thatoom, A.Srimahaphote, Prachinburi, 25140.

Calibrated at : Electrical and Electronic Standards Laboratory, Industrial Metrology and Testing Service Centre.
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Rd., A.Muang, Samutprakan 10280.

Instrument Calibrated :

Description : Integrating Sound Level Meter
Manufacturer : ACO
Model : 6226
Serial No. : 100146
Microphone : Type 7052NR No.78402
Preamplifier : -

Ambient Environment

Temperature : (23 ± 3) °C
Relative Humidity : (50 ± 15) %
Ambient Pressure : (101.325 ± 1.5) kPa

Standards used :

1. Band Pass Filter Stanford Research Systems SR 650 S/N 28712.
2. Condenser Microphone Brüel&Kjær 4180 S/N 2889871.
3. Decade Attenuator Ando AL-205 S/N 00464602.
4. Function/Arbitrary Waveform Generator Agilent 33220A S/N MY44042668.
5. Digital Function Synthesizer NF Electronic Instruments DF-193A S/N 122037.
6. Sound Calibrator Brüel&Kjær 4231 S/N 3015154.
7. Measuring Amplifier Brüel&Kjær 2636 S/N 1537484.

Date of Receipt : 14 Jan. 2025

Date of Calibration : 17-18 Feb. 2025

1 / 9

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BLMTC.002 Rev.5

8. Power Amplifier Brüel&Kjær 2706 S/N 1517650.
9. Speaker Tannoy Limited, Great Britain British Patent No. 215300.
10. Digital Multimeter Agilent 34401A S/N MY44005560.
11. Programmable Attenuator Tamagawa TPA-303A S/N 2212.

Calibration Procedure :

This instrument was calibrated by using calibration procedures no CP-102-02 and CP-102-03, which were based on IEC 61672-3 Electroacoustics - Sound Level Meters - Part 3 : Periodic tests (2013). These calibration procedures were related to the electrical and acoustic signal tests. The electrical signal test was carried out with the direct measurement method. The acoustic signal test was performed in an anechoic room with the comparison measurement method.

This instrument has been calibrated against standards maintained at the Electrical and Electronic Standards Laboratory (EEL), which are traceable to the International System of Units through the National Institute of Metrology (Thailand).

The information on actual reading is attached herewith and the uncertainty limits quoted refer to the measured values only.

The reported expanded uncertainty is based upon a standard uncertainty multiplied by a coverage factor k=2, providing a level of confidence of approximately 95%.

Date of Calibration : 17-18 Feb. 2025

2 / 9

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BLMTC.002 Rev.5

1. Absolute Sensitivity

Reference Acoustic Signal (dB)	Measured value (dB)		Deviation value (dB)	Acceptance limit Class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
	Before adjust	After adjust				
93.99	92.7	94.0	0.0	1.0	0.30	N/A

Note: The external calibration adjustment was firstly performed. The internal calibration adjustment was then completed at the display of 95.1 dB.

2. Self-generated noise

2.1 Normal test

Measured value (dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
23.1	0.10	N/A

2.2 The microphone of the sound level meter was replaced by electrical signal input device

Frequency	Measured value (dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Weighting			
A-Weight	22.5	0.10	N/A
C-Weight	27.6	0.10	N/A
Flat	30.1	0.10	N/A

Date of Calibration : 17-18 Feb. 2025

3 / 9

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BLMTC.002 Rev.5

3. Acoustical signal test of frequency weightings

Frequency (Hz)	Deviation from frequency response (dB)			Acceptance limit class 2 (\pm dB)	Uncertainty (\pm dB)	Maximum-permitted uncertainty of measurement (\pm dB)
	A-weight	C-weight	Flat			
125	0.7	0.5	0.0	1.5	0.45	0.6
1 000	0.2	0.1	0.1	1.0	0.45	0.6
8 000	-4.4	-4.2	-4.4	5.0	0.45	0.7

4. Electrical signal test of frequency weightings

Frequency (Hz)	Deviation from frequency response (dB)			Acceptance limit class 2 (\pm dB)	Uncertainty (\pm dB)	Maximum-permitted uncertainty of measurement (\pm dB)
	A-weight	C-weight	Flat			
63	0.3	0.1	0.1	2.0	0.20	0.6
125	0.1	0.1	1.3	1.5	0.20	0.6
250	0.1	0.1	0.1	1.5	0.20	0.6
500	0.1	0.0	0.0	1.5	0.20	0.6
1 000	0.0	0.0	0.0	1.0	0.20	0.6
2 000	-0.1	0.0	0.1	2.0	0.20	0.6
4 000	-0.4	-0.2	0.0	3.0	0.20	0.6
8 000	-0.3	-0.2	-0.1	5.0	0.20	0.7

Date of Calibration : 17-18 Feb. 2025

4 / 9

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FMLBL/MTC.002 Rev.5

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9009

Office/Laboratory
668 Mu 2 Tambon Bangpoojai, Amphoe Muang Samutprakarn,
Changwat Samutprakarn 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtg@tistr.or.th Website : www.tistr.or.th

Office
196 Phahonyothin Road, Ladyao, Chatuchak,
Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827

7. Level linearity on the reference level range

Anticipated value (dB)	Measured Value (dB)	Deviated value (dB)	Acceptance limit class 2 (\pm dB)	Uncertainty (\pm dB)	Maximum-permitted uncertainty of measurement (\pm dB)
122	121.8	-0.2	1.1	0.30	0.3
121	120.9	-0.1	1.1	0.30	0.3
120	119.9	-0.1	1.1	0.30	0.3
119	118.9	-0.1	1.1	0.30	0.3
114	113.9	-0.1	1.1	0.30	0.3
109	108.9	-0.1	1.1	0.30	0.3
104	103.9	-0.1	1.1	0.30	0.3
99	99.0	0.0	1.1	0.30	0.3
94	94.0	0.0	1.1	0.30	0.3
89	88.9	-0.1	1.1	0.30	0.3
84	84.1	0.1	1.1	0.30	0.3
79	78.9	-0.1	1.1	0.30	0.3
74	73.9	-0.1	1.1	0.30	0.3
69	68.9	-0.1	1.1	0.30	0.3
64	63.9	-0.1	1.1	0.30	0.3
59	58.8	-0.2	1.1	0.30	0.3
54	53.9	-0.1	1.1	0.30	0.3
49	48.9	-0.1	1.1	0.30	0.3
44	44.2	0.2	1.1	0.30	0.3
39	39.0	0.0	1.1	0.30	0.3
34	34.1	0.1	1.1	0.30	0.3
33	33.2	0.2	1.1	0.30	0.3

Date of Calibration : 17-18 Feb. 2025

6 / 9

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FMLBL/MTC.002 Rev.5

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9009

Office/Laboratory
668 Mu 2 Tambon Bangpoojai, Amphoe Muang Samutprakarn,
Changwat Samutprakarn 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtg@tistr.or.th Website : www.tistr.or.th

Office
196 Phahonyothin Road, Ladyao, Chatuchak,
Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827

5. Long-term stability

Time	Measured Value (dB)	Deviated value (dB)	Acceptance limit class 2 (\pm dB)	Uncertainty (\pm dB)	Maximum-permitted uncertainty of measurement (\pm dB)
Begin	94.0	0.0	0.3	0.10	0.1
End	94.0				

6. Frequency and time weightings at 1 kHz
6.1 Frequency weightings at 1 kHz

Frequency Weighting	Measured Value (dB)	Deviated value (dB)	Acceptance limit class 2 (\pm dB)	Uncertainty (\pm dB)	Maximum-permitted uncertainty of measurement (\pm dB)
A-weight	94.0	0.0	0.2	0.20	0.2
C-weight	94.0	0.0	0.2	0.20	0.2
Flat	94.1	0.1	0.2	0.20	0.2

6.2 Time weightings at 1 kHz

Frequency Weighting	Measured Value (dB)	Deviated value (dB)	Acceptance limit class 2 (\pm dB)	Uncertainty (\pm dB)	Maximum-permitted uncertainty of measurement (\pm dB)
Fast	94.0	0.0	0.1	0.20	0.2
Slow	94.0	0.0	0.1	0.20	0.2
Leq	94.0	0.0	0.1	0.20	0.2

Date of Calibration : 17-18 Feb. 2025

5 / 9

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FMLBL/MTC.002 Rev.5

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9009

Office/Laboratory
668 Mu 2 Tambon Bangpoojai, Amphoe Muang Samutprakarn,
Changwat Samutprakarn 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtg@tistr.or.th Website : www.tistr.or.th

Office
196 Phahonyothin Road, Ladyao, Chatuchak,
Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827

7. Level linearity on the reference level range

Anticipated value (dB)	Measured Value (dB)	Deviated value (dB)	Acceptance limit class 2 (\pm dB)	Uncertainty (\pm dB)	Maximum-permitted uncertainty of measurement (\pm dB)
32	32.3	0.3	1.1	0.30	0.3
31	31.4	0.4	1.1	0.30	0.3
30	30.4	0.4	1.1	0.30	0.3

8. Level linearity including the level range control

At reference sound level on the reference level range

Range	Anticipated value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (\pm dB)	Uncertainty (\pm dB)	Maximum-permitted uncertainty of measurement (\pm dB)
40-130	94.0	94.0	0.0	1.1	0.30	0.3
30-120	94.0	94.0	0.0	1.1	0.30	0.3
20-110	94.0	94.0	0.0	1.1	0.30	0.3
20-100	94.0	94.0	0.0	1.1	0.30	0.3

Date of Calibration : 17-18 Feb. 2025

7 / 9

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FMLBL/MTC.002 Rev.5

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9009

Office/Laboratory
668 Mu 2 Tambon Bangpoojai, Amphoe Muang Samutprakarn,
Changwat Samutprakarn 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtg@tistr.or.th Website : www.tistr.or.th

Office
196 Phahonyothin Road, Ladyao, Chatuchak,
Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827

8. Level linearity including the level range control

At reference level at 5 dB greater than the under-range on a level range

Range	Anticipated value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
40-130	45	45.0	0.0	1.1	0.30	0.3
30-120	35	35.0	0.0	1.1	0.30	0.3
20-110	25	25.8	0.8	1.1	0.30	0.3
20-100	25	25.8	0.8	1.1	0.30	0.3
20-90	25	25.6	0.6	1.1	0.30	0.3
20-80	25	25.7	0.7	1.1	0.30	0.3

9. Tone burst response

Time Weighting	Toneburst Duration, Tb (ms)	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Fast	200	115.8	-0.2	±1.0	0.20	0.3
	2	98.8	-0.2	+1.0; -2.5	0.20	0.3
	0.25	89.6	-0.4	+1.5; -5.0	0.20	0.3
Slow	200	109.4	-0.2	±1.0	0.20	0.3
	2	89.8	-0.2	+1.0; -5.0	0.20	0.3
SEL	200	109.9	-0.1	±1.0	0.20	0.3
	2	90.0	0.0	+1.0; -2.5	0.20	0.3
	0.25	80.9	-0.1	+1.5; -5.0	0.20	0.3

Date of Calibration : 17-18 Feb. 2025

8 / 9

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.5

 Head Office
 35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
 Changwat Pathumthani 12120, Thailand
 Tel. (66) 0 2577 9036
 Fax. (66) 0 2577 9009

 Office/Laboratory
 668 Mu 2 Tambon Bangpoojai, Amphoe Muang Samutprakan,
 Changwat Samutprakan 10280, Thailand
 Tel. (66) 0 2323 1672-80 ext. 115, 116
 (66) 08 3219 9440
 E-mail : mtc@tistr.or.th Website : www.tistr.or.th

 Office
 196 Phahonyothin Road, Ladysa, Chatuchak,
 Bangkok 10900, Thailand
 Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5237
 (66) 08 1889 6827

CALIBRATION CERTIFICATE

Submitted by : Integrated Research Center Company Limited.

Address : 122 Moo 2, T.Thatoom, A.Srimahaphote, Prachinburi, 25140.

Calibrated at : Electrical and Electronic Standards Laboratory, Industrial Metrology and Testing Service Centre.

Soi 1C, Bangpoo Industrial Estate, Sukhumvit Rd., A.Muang, Samutprakan 10280.

Instrument Calibrated :

Description : Sound Level Meter

Manufacturer : Delta OHM

Model : HD 2010UC

Serial No. : 11040842479

Microphone : Type UC-52 No.114674

Preamplifier : Delta Type HD2010PNE2 No.11001018

Ambient Environment

Temperature : (23 ± 3) °C

Relative Humidity : (50 ± 15) %

Ambient Pressure : (101.325±1.5) kPa

Standards used :

1. Band Pass Filter Stanford Research Systems SR 650 S/N 28712.
2. Condenser Microphone Brüel&Kjær 4180 S/N 2889871.
3. Decade Attenuator Ando AL-205 S/N 00464602.
4. Function/Arbitrary Waveform Generator Agilent 33220A S/N MY44042668.
5. Digital Function Synthesizer NF Electronic Instruments DF-193A S/N 122037.
6. Sound Calibrator Brüel&Kjær 4231 S/N 3015154.
7. Measuring Amplifier Brüel&Kjær 2636 S/N 1537484.

Date of Receipt : 14 Jan. 2025

Date of Calibration : 17-18 Feb. 2025

1 / 9

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.5

 Head Office
 35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
 Changwat Pathumthani 12120, Thailand
 Tel. (66) 0 2577 9036
 Fax. (66) 0 2577 9009

 Office/Laboratory
 668 Mu 2 Tambon Bangpoojai, Amphoe Muang Samutprakan,
 Changwat Samutprakan 10280, Thailand
 Tel. (66) 0 2323 1672-80 ext. 115, 116
 (66) 08 3219 9440
 E-mail : mtc@tistr.or.th Website : www.tistr.or.th

 Office
 196 Phahonyothin Road, Ladysa, Chatuchak,
 Bangkok 10900, Thailand
 Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5237
 (66) 08 1889 6827

10. Peak C sound level

Number of cycles in test signal	Anticipated value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Complete cycle	125.4	125.8	0.4	3.0	0.20	0.35
Positive half cycle	124.4	124.2	-0.2	2.0	0.20	0.35
Negative half cycle	124.4	124.2	-0.2	2.0	0.20	0.35

11. Overload indication

Measured value (dB)		Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)	
Positive one-half cycle	Negative one-half cycle	131.1	0.0	1.5	0.20	0.25

12. High-level stability

Time	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Begin	129.0	0.0	0.3	0.10	0.1
End	129.0				

 Calibrated by
 (Mr. Pannasit Phasingiri)

 Approved by :
 (Mr. Praswate Klauyapa)
 Director

Electrical and Electronic Standards Laboratory

Industrial Metrology and Testing Service Centre

Date of Calibration : 17-18 Feb. 2025

Date of Issue : 24 Feb. 2025

Ref : 2011268011400185009

End of Certificate

9 / 9

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.5

 Head Office
 35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
 Changwat Pathumthani 12120, Thailand
 Tel. (66) 0 2577 9036
 Fax. (66) 0 2577 9009

 Office/Laboratory
 668 Mu 2 Tambon Bangpoojai, Amphoe Muang Samutprakan,
 Changwat Samutprakan 10280, Thailand
 Tel. (66) 0 2323 1672-80 ext. 115, 116
 (66) 08 3219 9440
 E-mail : mtc@tistr.or.th Website : www.tistr.or.th

 Office
 196 Phahonyothin Road, Ladysa, Chatuchak,
 Bangkok 10900, Thailand
 Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5237
 (66) 08 1889 6827

8. Power Amplifier Brüel&Kjær 2706 S/N 1517650.
9. Speaker Tannoy Limited, Great Britain British Patent No. 215300.
10. Digital Multimeter Agilent 34401A S/N MY44005560.
11. Programmable Attenuator Tamagawa TPA-303A S/N 2212.

Calibration Procedure :

This instrument was calibrated by using calibration procedures no CP-102-02 and CP-102-03, which were based on IEC 61672-3 Electroacoustics - Sound Level Meters - Part 3 : Periodic tests (2013). These calibration procedures were related to the electrical and acoustic signal tests. The electrical signal test was carried out with the direct measurement method. The acoustic signal test was performed in an anechoic room with the comparison measurement method.

This instrument has been calibrated against standards maintained at the Electrical and Electronic Standards Laboratory (EEL), which are traceable to the International System of Units through the National Institute of Metrology (Thailand).

The information on actual reading is attached herewith and the uncertainty limits quoted refer to the measured values only.

The reported expanded uncertainty is based upon a standard uncertainty multiplied by a coverage factor k=2, providing a level of confidence of approximately 95%.

Date of Calibration : 17-18 Feb. 2025

2 / 9

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.5

 Head Office
 35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
 Changwat Pathumthani 12120, Thailand
 Tel. (66) 0 2577 9036
 Fax. (66) 0 2577 9009

 Office/Laboratory
 668 Mu 2 Tambon Bangpoojai, Amphoe Muang Samutprakan,
 Changwat Samutprakan 10280, Thailand
 Tel. (66) 0 2323 1672-80 ext. 115, 116
 (66) 08 3219 9440
 E-mail : mtc@tistr.or.th Website : www.tistr.or.th

 Office
 196 Phahonyothin Road, Ladysa, Chatuchak,
 Bangkok 10900, Thailand
 Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5237
 (66) 08 1889 6827

1. Absolute Sensitivity

Reference Acoustic Signal (dB)	Measured value (dB)		Deviation value (dB)	Acceptance limit Class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
	Before adjust	After adjust				
93.95	93.3	94.0	0.1	1.0	0.30	N/A

Note: The external calibration adjustment was firstly performed. The internal calibration adjustment was then completed at the display of 94.0 dB.

2. Self-generated noise

2.1 Normal test

Measured value (dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
19.6	0.10	N/A

2.2 The microphone of the sound level meter was replaced by electrical signal input device

Frequency Weighting	Measured value (dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
A-Weight	18.3	0.10	N/A
C-Weight	24.5	0.20	N/A
Flat	26.9	0.30	N/A

Date of Calibration : 17-18 Feb. 2025

3 / 9

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FMBL.MTC.002 Rev.5

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang, Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9009

Office/Laboratory
668 Mu 2 Tambon Bangpoornai, Amphoe Muang Samutprakan, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtg@tistr.or.th Website : www.tistr.or.th

Office
196 Phahonyothin Road, Ladyao, Chatuchak, Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827

5. Long-term stability

Time	Measured Value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Begin	94.0	0.0	0.3	0.10	0.1
End	94.0				

6. Frequency and time weightings at 1 kHz

6.1 Frequency weightings at 1 kHz

Frequency Weighting	Measured Value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
A-weight	94.0	0.0	0.2	0.20	0.2
C-weight	94.0	0.0	0.2	0.20	0.2
Flat	94.1	0.1	0.2	0.20	0.2

6.2 Time weightings at 1 kHz

Frequency Weighting	Measured Value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Fast	94.0	0.0	0.1	0.20	0.2
Slow	94.0	0.0	0.1	0.20	0.2
Leq	94.0	0.0	0.1	0.20	0.2

Date of Calibration : 17-18 Feb. 2025

5 / 9

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FMBL.MTC.002 Rev.5

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang, Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9009

Office/Laboratory
668 Mu 2 Tambon Bangpoornai, Amphoe Muang Samutprakan, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtg@tistr.or.th Website : www.tistr.or.th

Office
196 Phahonyothin Road, Ladyao, Chatuchak, Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827

3. Acoustical signal test of frequency weightings

Frequency (Hz)	Deviation from frequency response (dB)			Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
	A-weight	C-weight	Flat			
125	0.4	0.3	0.2	1.5	0.45	0.6
1 000	-0.5	-0.5	-0.5	1.0	0.45	0.6
8 000	-4.0	-3.9	-4.0	5.0	0.45	0.7

4. Electrical signal test of frequency weightings

Frequency (Hz)	Deviation from frequency response (dB)			Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
	A-weight	C-weight	Flat			
63	-0.1	-0.2	-0.3	2.0	0.20	0.6
125	-0.1	-0.1	-0.2	1.5	0.20	0.6
250	0.0	-0.1	-0.1	1.5	0.20	0.6
500	0.0	0.0	0.0	1.5	0.20	0.6
1 000	0.0	0.0	0.0	1.0	0.20	0.6
2 000	0.0	0.1	0.1	2.0	0.20	0.6
4 000	0.1	0.1	0.1	3.0	0.20	0.6
8 000	0.1	0.1	0.1	5.0	0.20	0.7

Date of Calibration : 17-18 Feb. 2025

4 / 9

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FMBL.MTC.002 Rev.5

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang, Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9009

Office/Laboratory
668 Mu 2 Tambon Bangpoornai, Amphoe Muang Samutprakan, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtg@tistr.or.th Website : www.tistr.or.th

Office
196 Phahonyothin Road, Ladyao, Chatuchak, Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827

7. Level linearity on the reference level range

Anticipated value (dB)	Measured Value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
120	120.0	0.0	1.1	0.30	0.3
119	119.0	0.0	1.1	0.30	0.3
114	114.0	0.0	1.1	0.30	0.3
109	109.0	0.0	1.1	0.30	0.3
104	104.0	0.0	1.1	0.30	0.3
99	99.0	0.0	1.1	0.30	0.3
94	94.0	0.0	1.1	0.30	0.3
89	89.0	0.0	1.1	0.30	0.3
84	84.0	0.0	1.1	0.30	0.3
79	79.0	0.0	1.1	0.30	0.3
74	74.0	0.0	1.1	0.30	0.3
69	69.0	0.0	1.1	0.30	0.3
64	64.0	0.0	1.1	0.30	0.3
59	59.0	0.0	1.1	0.30	0.3
54	54.0	0.0	1.1	0.30	0.3
49	49.0	0.0	1.1	0.30	0.3
44	44.0	0.0	1.1	0.30	0.3
43	43.0	0.0	1.1	0.30	0.3
42	42.1	0.1	1.1	0.30	0.3

Date of Calibration : 17-18 Feb. 2025

6 / 9

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FMBL.MTC.002 Rev.5

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang, Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9009

Office/Laboratory
668 Mu 2 Tambon Bangpoornai, Amphoe Muang Samutprakan, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtg@tistr.or.th Website : www.tistr.or.th

Office
196 Phahonyothin Road, Ladyao, Chatuchak, Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827



7. Level linearity on the reference level range

Anticipated value (dB)	Measured Value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
41	41.1	0.1	1.1	0.30	0.3
40	40.1	0.1	1.1	0.30	0.3
39	39.1	0.1	1.1	0.30	0.3

8. Level linearity including the level range control

At reference sound level on the reference level range

Range	Anticipated value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
60-140	94.0	94.0	0.0	1.1	0.30	0.3
50-130	94.0	94.0	0.0	1.1	0.30	0.3
40-120	94.0	94.0	0.0	1.1	0.30	0.3
30-110	94.0	94.0	0.0	1.1	0.30	0.3
20-100	94.0	94.0	0.0	1.1	0.30	0.3

Date of Calibration : 17-18 Feb. 2025

7 / 9

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.5

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9039

Office/Laboratory
668 Mu 2 Tambon Bangpoo, Amphoe Muang Samutprakan,
Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtg@tistr.or.th Website : www.tistr.or.th

Office
196 Phahonyothin Road, Ladysao, Chatuchak,
Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827



10. Peak C sound level

Number of cycles in test signal	Anticipated value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Complete cycle	135.4	135.3	-0.1	3.0	0.20	0.35
Positive half cycle	134.4	134.2	-0.2	2.0	0.20	0.35
Negative half cycle	134.4	134.2	-0.2	2.0	0.20	0.35

11. Overload indication

Measured value (dB)		Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Positive one-half cycle	Negative one-half cycle				
140.5	140.5	0.0	1.5	0.20	0.25

12. High-level stability

Time	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Begin	139.0	0.0	0.3	0.10	0.1
End	139.0				

Calibrated by :
(Mr. Pannasit Phasingri)

Approved by :
(Mr. Pravee Klungsapa)

Electrical and Electronic Standards Laboratory

Industrial Metrology and Testing Service Centre

Date of Calibration : 17-18 Feb. 2025

Date of Issue : 24 Feb. 2025

Ref : 2011268011400185012

End of Certificate

9 / 9

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.5

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9039

Office/Laboratory
668 Mu 2 Tambon Bangpoo, Amphoe Muang Samutprakan,
Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtg@tistr.or.th Website : www.tistr.or.th

Office
196 Phahonyothin Road, Ladysao, Chatuchak,
Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827



8. Level linearity including the level range control

At reference level at 5 dB greater than the under-range on a level range

Range	Anticipated value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
60-140	65	65.0	0.0	1.1	0.30	0.3
50-130	55	55.0	0.0	1.1	0.30	0.3
40-120	45	45.0	0.0	1.1	0.30	0.3
30-110	35	35.2	0.2	1.1	0.30	0.3
20-100	25	25.3	0.3	1.1	0.30	0.3

9. Tone burst response

Time Weighting	Toneburst Duration, Tb (ms)	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Fast	200	115.8	-0.2	±1.0	0.20	0.3
	2	98.8	-0.2	+1.0; -2.5	0.20	0.3
	0.25	89.6	-0.4	+1.5; -5.0	0.20	0.3
Slow	200	109.4	-0.2	±1.0	0.20	0.3
	2	89.8	-0.2	+1.0; -5.0	0.20	0.3
SEL	200	109.9	-0.1	±1.0	0.20	0.3
	2	90.0	0.0	+1.0; -2.5	0.20	0.3
	0.25	80.9	-0.1	+1.5; -5.0	0.20	0.3

Date of Calibration : 17-18 Feb. 2025

8 / 9

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.5

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9039

Office/Laboratory
668 Mu 2 Tambon Bangpoo, Amphoe Muang Samutprakan,
Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtg@tistr.or.th Website : www.tistr.or.th

Office
196 Phahonyothin Road, Ladysao, Chatuchak,
Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827



CALIBRATION CERTIFICATE

Submitted by : Integrated Research Center Company Limited.

Address : 122 Moo 2, T.Thatoom, A.Srimahaphote, Prachinburi, 25140.

Calibrated at : Electrical and Electronic Standards Laboratory, Industrial Metrology and Testing Service Centre.

Soi 1C, Bangpoo Industrial Estate, Sukhumvit Rd., A.Muang, Samutprakan 10280.

Instrument Calibrated :

Description : Sound Level Meter

Manufacturer : Rion

Model : NI-42

Serial No. : 00433730

Microphone : Type UC-52 No.144953

Preamplifier : Type NH-24 No.33780

Standards used :

- Band Pass Filter Stanford Research Systems SR 650 S/N 28712.
- Condenser Microphone Brüel&Kjær 4180 S/N 2889871.
- Decade Attenuator Ando AL-205 S/N 00464602.
- Function/Arbitrary Waveform Generator Agilent 33220A S/N MY44042668.
- Digital Function Synthesizer NF Electronic Instruments DF-193A S/N 122037.
- Sound Calibrator Brüel&Kjær 4231 S/N 3015154.
- Measuring Amplifier Brüel&Kjær 2636 S/N 1537484.

Date of Receipt : 14 Jan. 2025

Date of Calibration : 17-18 Feb. 2025

1 / 9

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.5

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9039

Office/Laboratory
668 Mu 2 Tambon Bangpoo, Amphoe Muang Samutprakan,
Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtg@tistr.or.th Website : www.tistr.or.th

Office
196 Phahonyothin Road, Ladysao, Chatuchak,
Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827

8. Power Amplifier Brüel&Kjær 2706 S/N 1517650.
9. Speaker Tannoy Limited, Great Britain British Patent No. 215300.
10. Digital Multimeter Agilent 34401A S/N MY44005560.
11. Programmable Attenuator Tamagawa TPA-303A S/N 2212.

Calibration Procedure :

This instrument was calibrated by using calibration procedures no CP-102-02 and CP-102-03, which were based on IEC 61672-3 Electroacoustics - Sound Level Meters - Part 3 : Periodic tests (2013). These calibration procedures were related to the electrical and acoustic signal tests. The electrical signal test was carried out with the direct measurement method. The acoustic signal test was performed in an anechoic room with the comparison measurement method.

This instrument has been calibrated against standards maintained at the Electrical and Electronic Standards Laboratory (EEL), which are traceable to the International System of Units through the National Institute of Metrology (Thailand).

The information on actual reading is attached herewith and the uncertainty limits quoted refer to the measured values only.

The reported expanded uncertainty is based upon a standard uncertainty multiplied by a coverage factor $k=2$, providing a level of confidence of approximately 95%.

Date of Calibration : 17-18 Feb. 2025

2 / 9

The results relate only to the items tested/calibrated or value assigned. Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FMBL.MTC.002 Rev.5

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9009

Office/Laboratory
668 Mu 2 Tambon Bangpoomai, Amphoe Muang Samutprakan,
Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtic@tistr.or.th Website : www.tistr.or.th

Office
196 Phahonyothin Road, Ladysao, Chatuchak,
Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827

3. Acoustical signal test of frequency weightings

Frequency (Hz)	Deviation from frequency response (dB)			Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
	A-weight	C-weight	Flat			
125	0.1	0.3	0.0	1.5	0.45	0.6
1 000	0.1	0.0	0.1	1.0	0.45	0.6
8 000	-4.6	-4.4	-4.7	5.0	0.45	0.7

4. Electrical signal test of frequency weightings

Frequency (Hz)	Deviation from frequency response (dB)			Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
	A-weight	C-weight	Flat			
63	0.0	0.0	0.1	2.0	0.20	0.6
125	0.0	0.1	0.1	1.5	0.20	0.6
250	0.0	0.1	0.1	1.5	0.20	0.6
500	0.0	0.0	0.0	1.5	0.20	0.6
1 000	0.0	0.0	0.0	1.0	0.20	0.6
2 000	0.0	0.1	0.1	2.0	0.20	0.6
4 000	0.0	0.1	0.1	3.0	0.20	0.6
8 000	0.1	0.1	0.1	5.0	0.20	0.7

Date of Calibration : 17-18 Feb. 2025

4 / 9

The results relate only to the items tested/calibrated or value assigned. Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FMBL.MTC.002 Rev.5

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9009

Office/Laboratory
668 Mu 2 Tambon Bangpoomai, Amphoe Muang Samutprakan,
Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtic@tistr.or.th Website : www.tistr.or.th

Office
196 Phahonyothin Road, Ladysao, Chatuchak,
Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827

1. Absolute Sensitivity

Reference Acoustic Signal (dB)	Measured value (dB)		Deviation value (dB)	Acceptance limit Class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
	Before adjust	After adjust				
93.95	93.8	113.9	20.0	1.0	0.30	N/A

Note: The external calibration adjustment was firstly performed. The internal calibration adjustment was then completed at the display of 124.0 dB.

2. Self-generated noise

2.1 Normal test

Measured value (dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
17.9	0.10	N/A

2.2 The microphone of the sound level meter was replaced by electrical signal input device

Frequency Weighting	Measured value (dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
A-Weight	14.3	0.70	N/A
C-Weight	19.4	0.70	N/A
Flat	25.1	0.30	N/A

Date of Calibration : 17-18 Feb. 2025

3 / 9

The results relate only to the items tested/calibrated or value assigned. Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FMBL.MTC.002 Rev.5

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9009

Office/Laboratory
668 Mu 2 Tambon Bangpoomai, Amphoe Muang Samutprakan,
Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtic@tistr.or.th Website : www.tistr.or.th

Office
196 Phahonyothin Road, Ladysao, Chatuchak,
Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827

5. Long-term stability

Time	Measured Value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Begin	94.0	0.0	0.3	0.10	0.1
End	94.0				

6. Frequency and time weightings at 1 kHz

6.1 Frequency weightings at 1 kHz

Frequency Weighting	Measured Value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
A-weight	94.0	0.0	0.2	0.20	0.2
C-weight	94.0	0.0	0.2	0.20	0.2
Flat	94.1	0.1	0.2	0.20	0.2

6.2 Time weightings at 1 kHz

Frequency Weighting	Measured Value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Fast	94.0	0.0	0.1	0.20	0.2
Slow	94.0	0.0	0.1	0.20	0.2
Leq	94.0	0.0	0.1	0.20	0.2

Date of Calibration : 17-18 Feb. 2025

5 / 9

The results relate only to the items tested/calibrated or value assigned. Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FMBL.MTC.002 Rev.5

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9009

Office/Laboratory
668 Mu 2 Tambon Bangpoomai, Amphoe Muang Samutprakan,
Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtic@tistr.or.th Website : www.tistr.or.th

Office
196 Phahonyothin Road, Ladysao, Chatuchak,
Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827

7. Level linearity on the reference level range

Anticipated value (dB)	Measured Value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
137	137.1	0.1	1.1	0.64	0.3
136	136.1	0.1	1.1	0.69	0.3
135	135.0	0.0	1.1	0.58	0.3
133	133.0	0.0	1.1	0.64	0.3
132	132.0	0.0	1.1	0.64	0.3
131	131.0	0.0	1.1	0.64	0.3
130	130.0	0.0	1.1	0.64	0.3
129	129.0	0.0	1.1	2.90	0.3
124	124.0	0.0	1.1	2.90	0.3
119	119.0	0.0	1.1	2.90	0.3
114	114.0	0.0	1.1	2.90	0.3
109	109.0	0.0	1.1	2.90	0.3
104	104.0	0.0	1.1	2.90	0.3
99	99.0	0.0	1.1	0.30	0.3
94	94.0	0.0	1.1	0.30	0.3
89	89.0	0.0	1.1	0.30	0.3
84	84.1	0.1	1.1	0.30	0.3
79	79.0	0.0	1.1	0.30	0.3
74	74.0	0.0	1.1	0.30	0.3
69	69.0	0.0	1.1	0.30	0.3
64	64.0	0.0	1.1	0.30	0.3
59	58.9	-0.1	1.1	0.30	0.3

Date of Calibration : 17-18 Feb. 2025

6/9

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FMBL.MTC.002 Rev.5

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9009

Office/Laboratory
668 Mu 2 Tambon Bangpoornai, Amphoe Muang Samutprakan,
Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtc@tistr.or.th Website : www.tistr.or.th

Office
136 Phahonyothin Road, Ladysao, Chatuchak,
Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827

8. Level linearity including the level range control

At reference level at 5 dB greater than the under-range on a level range

Range	Anticipated value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
30-130	25	25.0	0.0	1.1	0.30	0.3

9. Tone burst response

Time Weighting	Toneburst Duration, T _b (ms)	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Fast	200	126.0	0.0	±1.0	0.20	0.3
	2	108.9	-0.1	+1.0; -2.5	0.20	0.3
	0.25	100.0	0.0	+1.5; -5.0	0.20	0.3
Slow	200	119.5	-0.1	±1.0	0.20	0.3
	2	100.0	0.0	+1.0; -5.0	0.20	0.3

Date of Calibration : 17-18 Feb. 2025

8/9

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FMBL.MTC.002 Rev.5

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9009

Office/Laboratory
668 Mu 2 Tambon Bangpoornai, Amphoe Muang Samutprakan,
Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtc@tistr.or.th Website : www.tistr.or.th

Office
136 Phahonyothin Road, Ladysao, Chatuchak,
Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827

7. Level linearity on the reference level range (cont.)

Anticipated value (dB)	Measured Value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
54	53.9	-0.1	1.1	0.30	0.3
49	48.9	-0.1	1.1	0.30	0.3
44	44.0	0.0	1.1	0.30	0.3
39	38.9	-0.1	1.1	0.30	0.3
34	33.9	-0.1	1.1	0.30	0.3
29	29.0	0.0	1.1	0.30	0.3
28	27.9	-0.1	1.1	0.30	0.3
27	26.9	-0.1	1.1	0.30	0.3
26	25.9	-0.1	1.1	0.30	0.3
25	24.9	-0.1	1.1	0.30	0.3

8. Level linearity including the level range control

At reference sound level on the reference level range

Range	Anticipated value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
30-130	94.0	94.0	0.0	1.1	0.30	0.3

Date of Calibration : 17-18 Feb. 2025

7/9

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FMBL.MTC.002 Rev.5

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9009

Office/Laboratory
668 Mu 2 Tambon Bangpoornai, Amphoe Muang Samutprakan,
Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtc@tistr.or.th Website : www.tistr.or.th

Office
136 Phahonyothin Road, Ladysao, Chatuchak,
Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827

10. Peak C sound level

Number of cycles in test signal	Anticipated value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Complete cycle	125.4	125.5	0.1	3.0	0.20	0.35
Positive half cycle	124.4	124.1	-0.3	2.0	0.20	0.35
Negative half cycle	124.4	124.1	-0.3	2.0	0.20	0.35

11. Overload indication

Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)	
Positive one-half cycle	Negative one-half cycle	0.0	1.5	0.55	0.25
135.4	135.4				

12. High-level stability

Time	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Begin	129.0	0.0	0.3	0.10	0.1
End	129.0				

Calibrated by :
(Mr. Pannasit Phasingari)

Approved by :
(Mr. Prasante Kloaypa)
Director

Electrical and Electronic Standards Laboratory

Date of Calibration : 17-18 Feb. 2025

Industrial Metrology and Testing Service Centre

Date of Issue : 24 Feb. 2025

Ref : 2011268011400185010

End of Certificate

9/9

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FMBL.MTC.002 Rev.5

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9009

Office/Laboratory
668 Mu 2 Tambon Bangpoornai, Amphoe Muang Samutprakan,
Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtc@tistr.or.th Website : www.tistr.or.th

Office
136 Phahonyothin Road, Ladysao, Chatuchak,
Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827

CALIBRATION CERTIFICATE
Submitted by : Integrated Research Center Company Limited.

Address : 122 Moo 2, T.Thatoom, A.Srimahaphote, Prachinburi, 25140.

Calibrated at : Electrical and Electronic Standards Laboratory, Industrial Metrology and Testing Service Centre.
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Rd., A.Muang, Samutprakan 10280.

Instrument Calibrated :

Description : Sound Level Meter

Manufacturer : Rion

Model : NL-42

Serial No. : 00646442

Microphone : Type UC-52 No.142301

Preamplifier : Type NH-24 No.22410

Ambient Environment

Temperature : (23 ± 3) °C

Relative Humidity : (50 ± 15) %

Ambient Pressure : (101.325±1.5) kPa

Standards used :

1. Band Pass Filter Stanford Research Systems SR 650 S/N 28712.
2. Condenser Microphone Brüel&Kjær 4180 S/N 2889871.
3. Decade Attenuator Ando AL-205 S/N 00464602.
4. Function/Arbitrary Waveform Generator Agilent 33220A S/N MY44042668.
5. Digital Function Synthesizer NF Electronic Instruments DF-193A S/N 122037.
6. Sound Calibrator Bruel&Kjaer 4231 S/N 3015154.
7. Measuring Amplifier Brüel&Kjær 2636 S/N 1537484.

Date of Receipt : 14 Jan. 2025

Date of Calibration : 17-18 Feb. 2025

1/9

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FMBL/MTC.002 Rev.5

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9009

Office/Laboratory
668 Mu 2 Tambon Bangpoornai, Amphoe Muang Samutprakan,
Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtg@tistr.or.th Website : www.tistr.or.th

Office
196 Phahonyothin Road, Ladyao, Chatuchak,
Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827

1. Absolute Sensitivity

Reference Acoustic Signal (dB)	Measured value (dB)		Deviation value (dB)	Acceptance limit Class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
	Before adjust	After adjust				
93.95	93.6	113.9	20.0	1.0	0.30	N/A

Note: The external calibration adjustment was firstly performed. The internal calibration adjustment was then completed at the display of 124.3 dB.

2. Self-generated noise
2.1 Normal test

Measured value (dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
16.9	0.10	N/A

2.2 The microphone of the sound level meter was replaced by electrical signal input device

Frequency Weighting	Measured value (dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
A-Weight	13.1	0.10	N/A
C-Weight	18.5	0.10	N/A
Flat	24.4	0.10	N/A

Date of Calibration : 17-18 Feb. 2025

3/9

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FMBL/MTC.002 Rev.5

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9009

Office/Laboratory
668 Mu 2 Tambon Bangpoornai, Amphoe Muang Samutprakan,
Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtg@tistr.or.th Website : www.tistr.or.th

Office
196 Phahonyothin Road, Ladyao, Chatuchak,
Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827

8. Power Amplifier Brüel&Kjær 2706 S/N 1517650.
9. Speaker Tannoy Limited, Great Britain British Patent No. 215300.
10. Digital Multimeter Agilent 34401A S/N MY44005560.
11. Programmable Attenuator Tamagawa TPA-303A S/N 2212.

Calibration Procedure :

This instrument was calibrated by using calibration procedures no CP-102-02 and CP-102-03, which were based on IEC 61672-3 Electroacoustics - Sound Level Meters - Part 3 : Periodic tests (2013). These calibration procedures were related to the electrical and acoustic signal tests. The electrical signal test was carried out with the direct measurement method. The acoustic signal test was performed in an anechoic room with the comparison measurement method.

This instrument has been calibrated against standards maintained at the Electrical and Electronic Standards Laboratory (EEL), which are traceable to the International System of Units through the National Institute of Metrology (Thailand).

The information on actual reading is attached herewith and the uncertainty limits quoted refer to the measured values only.

The reported expanded uncertainty is based upon a standard uncertainty multiplied by a coverage factor $k=2$, providing a level of confidence of approximately 95%.

Date of Calibration : 17-18 Feb. 2025

2/9

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FMBL/MTC.002 Rev.5

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9009

Office/Laboratory
668 Mu 2 Tambon Bangpoornai, Amphoe Muang Samutprakan,
Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtg@tistr.or.th Website : www.tistr.or.th

Office
196 Phahonyothin Road, Ladyao, Chatuchak,
Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827

3. Acoustical signal test of frequency weightings

Frequency (Hz)	Deviation from frequency response (dB)			Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
	A-weight	C-weight	Flat			
125	0.8	0.2	0.0	1.5	0.45	0.6
1 000	0.0	0.0	0.0	1.0	0.45	0.6
8 000	-2.0	-2.0	-2.1	5.0	0.45	0.7

4. Electrical signal test of frequency weightings

Frequency (Hz)	Deviation from frequency response (dB)			Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
	A-weight	C-weight	Flat			
63	-0.1	0.0	0.0	2.0	0.20	0.6
125	-0.1	0.0	0.0	1.5	0.20	0.6
250	0.0	0.0	0.0	1.5	0.20	0.6
500	0.0	0.0	0.0	1.5	0.20	0.6
1 000	0.0	0.0	0.0	1.0	0.20	0.6
2 000	0.0	0.0	0.0	2.0	0.20	0.6
4 000	0.0	0.0	0.0	3.0	0.20	0.6
8 000	0.0	0.0	0.0	5.0	0.20	0.7

Date of Calibration : 17-18 Feb. 2025

4/9

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FMBL/MTC.002 Rev.5

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9009

Office/Laboratory
668 Mu 2 Tambon Bangpoornai, Amphoe Muang Samutprakan,
Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtg@tistr.or.th Website : www.tistr.or.th

Office
196 Phahonyothin Road, Ladyao, Chatuchak,
Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827

5. Long-term stability

Time	Measured Value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Begin	94.0	0.0	0.3	0.10	0.1
End	94.0				

6. Frequency and time weightings at 1 kHz
6.1 Frequency weightings at 1 kHz

Frequency Weighting	Measured Value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
A-weight	94.0	0.0	0.2	0.20	0.2
C-weight	94.0	0.0	0.2	0.20	0.2
Flat	94.1	0.1	0.2	0.20	0.2

6.2 Time weightings at 1 kHz

Frequency Weighting	Measured Value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Fast	94.0	0.0	0.1	0.20	0.2
Slow	94.0	0.0	0.1	0.20	0.2
Leq	94.0	0.0	0.1	0.20	0.2

Date of Calibration : 17-18 Feb. 2025

5 / 9

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FMBL.MTC.002 Rev.5

Head Office
 35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang, Changwat Pathumthani 12120, Thailand
 Tel. (66) 0 2577 9036
 Fax. (66) 0 2577 9009

Office/Laboratory
 668 Mu 2 Tambon Bangpoornai, Amphoe Muang Samutprakan, Changwat Samutprakan 10280, Thailand
 Tel. (66) 0 2323 1672-80 ext. 115, 116
 (66) 08 3219 9440
 E-mail : mtic@tistr.or.th Website : www.tistr.or.th

Office
 196 Phahonyothin Road, Ladysao, Chatuchak, Bangkok 10900, Thailand
 Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
 (66) 08 1889 6827

7. Level linearity on the reference level range (cont.)

Anticipated value (dB)	Measured Value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
54	54.0	0.0	1.1	0.30	0.3
49	48.9	-0.1	1.1	0.30	0.3
44	43.9	-0.1	1.1	0.30	0.3
39	38.9	-0.1	1.1	0.30	0.3
34	34.0	0.0	1.1	0.30	0.3
29	28.9	-0.1	1.1	0.30	0.3
28	27.9	-0.1	1.1	0.30	0.3
27	26.9	-0.1	1.1	0.30	0.3
26	25.9	-0.1	1.1	0.30	0.3
25	24.9	-0.1	1.1	0.30	0.3

8. Level linearity including the level range control

At reference sound level on the reference level range

Range	Anticipated value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
30-130	94.0	94.0	0.0	1.1	0.30	0.3

Date of Calibration : 17-18 Feb. 2025

7 / 9

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FMBL.MTC.002 Rev.5

Head Office
 35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang, Changwat Pathumthani 12120, Thailand
 Tel. (66) 0 2577 9036
 Fax. (66) 0 2577 9009

Office/Laboratory
 668 Mu 2 Tambon Bangpoornai, Amphoe Muang Samutprakan, Changwat Samutprakan 10280, Thailand
 Tel. (66) 0 2323 1672-80 ext. 115, 116
 (66) 08 3219 9440
 E-mail : mtic@tistr.or.th Website : www.tistr.or.th

Office
 196 Phahonyothin Road, Ladysao, Chatuchak, Bangkok 10900, Thailand
 Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
 (66) 08 1889 6827

7. Level linearity on the reference level range

Anticipated value (dB)	Measured Value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
137	136.6	-0.4	1.1	0.30	0.3
136	135.6	-0.4	1.1	0.30	0.3
135	134.7	-0.3	1.1	0.30	0.3
133	132.8	-0.2	1.1	0.30	0.3
132	131.8	-0.2	1.1	0.30	0.3
131	130.9	-0.1	1.1	0.30	0.3
130	129.9	-0.1	1.1	0.30	0.3
129	128.9	-0.1	1.1	0.30	0.3
124	124.0	0.0	1.1	0.30	0.3
119	119.0	0.0	1.1	0.30	0.3
114	114.0	0.0	1.1	0.30	0.3
109	109.0	0.0	1.1	0.30	0.3
104	104.0	0.0	1.1	0.30	0.3
99	99.0	0.0	1.1	0.30	0.3
94	94.0	0.0	1.1	0.30	0.3
89	89.0	0.0	1.1	0.30	0.3
84	84.0	0.0	1.1	0.30	0.3
79	78.9	-0.1	1.1	0.30	0.3
74	74.0	0.0	1.1	0.30	0.3
69	68.9	-0.1	1.1	0.30	0.3
64	64.0	0.0	1.1	0.30	0.3
59	58.9	-0.1	1.1	0.30	0.3

Date of Calibration : 17-18 Feb. 2025

6 / 9

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FMBL.MTC.002 Rev.5

Head Office
 35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang, Changwat Pathumthani 12120, Thailand
 Tel. (66) 0 2577 9036
 Fax. (66) 0 2577 9009

Office/Laboratory
 668 Mu 2 Tambon Bangpoornai, Amphoe Muang Samutprakan, Changwat Samutprakan 10280, Thailand
 Tel. (66) 0 2323 1672-80 ext. 115, 116
 (66) 08 3219 9440
 E-mail : mtic@tistr.or.th Website : www.tistr.or.th

Office
 196 Phahonyothin Road, Ladysao, Chatuchak, Bangkok 10900, Thailand
 Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
 (66) 08 1889 6827

8. Level linearity including the level range control

At reference level at 5 dB greater than the under-range on a level range

Range	Anticipated value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
30-130	25	25.0	0.0	1.1	0.30	0.3

9. Tone burst response

Time Weighting	Toneburst Duration, Tb (ms)	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Fast	200	126.0	0.0	±1.0	0.20	0.3
	2	108.9	-0.1	+1.0; -2.5	0.20	0.3
	0.25	100.0	0.0	+1.5; -5.0	0.20	0.3
Slow	200	119.5	-0.1	±1.0	0.20	0.3
	2	100.0	0.0	+1.0; -5.0	0.20	0.3

Date of Calibration : 17-18 Feb. 2025

8 / 9

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FMBL.MTC.002 Rev.5

Head Office
 35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang, Changwat Pathumthani 12120, Thailand
 Tel. (66) 0 2577 9036
 Fax. (66) 0 2577 9009

Office/Laboratory
 668 Mu 2 Tambon Bangpoornai, Amphoe Muang Samutprakan, Changwat Samutprakan 10280, Thailand
 Tel. (66) 0 2323 1672-80 ext. 115, 116
 (66) 08 3219 9440
 E-mail : mtic@tistr.or.th Website : www.tistr.or.th

Office
 196 Phahonyothin Road, Ladysao, Chatuchak, Bangkok 10900, Thailand
 Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
 (66) 08 1889 6827



10. Peak C sound level


Number of cycles in test signal	Anticipated value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Complete cycle	125.4	125.5	0.1	3.0	0.20	0.35
Positive half cycle	124.4	124.1	-0.3	2.0	0.20	0.35
Negative half cycle	124.4	124.1	-0.3	2.0	0.20	0.35

11. Overload indication

Measured value (dB)		Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Positive one-half cycle	Negative one-half cycle				
135.4	135.4	0.0	1.5	0.55	0.25

12. High-level stability

Time	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Begin	129.0	0.0	0.3	0.10	0.1
End	129.0				

Calibrated by: 
(Mr. Pannasit Phasingsri)

Approved by: 
(Mr. Pravee Klusaypa)
Director
Electrical and Electronic Standards Laboratory
Industrial Metrology and Testing Service Centre
Ref: 2011268011400185011

Date of Calibration : 17-18 Feb. 2025
Date of Issue : 24 Feb. 2025

End of Certificate

9 / 9

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FMBL.MTC.002 Rev.5



CALIBRATION CERTIFICATE

Submitted by : Integrated Research Center Company Limited.
Address : 122 Moo 2, T.Thatoom, A.Srimahaphote, Prachinburi 25140.
Calibrated at : Electrical and Electronic Standards Laboratory, Industrial Metrology and Testing Service Centre.
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Rd., A.Muang, Samutprakan 10280.

Instrument Calibrated :

Description : Sound Level Meter
Manufacturer : ACO
Model : 6236
Serial No. : 192014
Microphone : 7052NR No.73303
Preamplifier : -

Ambient Environment

Temperature : (23 ± 3) °C
Relative Humidity : (50 ± 15) %
Ambient Pressure : (101.325 ± 1.5) kPa

Standards used :

- Band Pass Filter Stanford Research Systems SR 650 S/N 28712.
- Condenser Microphone Brüel&Kjær 4180 S/N 2889871.
- Decade Attenuator Ando AL-205 S/N 00464602.
- Function/Arbitrary Waveform Generator Agilent 33220A S/N MY44042668.
- Digital Function Synthesizer NF Electronic Instruments DF-193A S/N 122037.
- Sound Calibrator Brüel&Kjær 4231 S/N 3015154.
- Measuring Amplifier Brüel&Kjær 2636 S/N 1537484.

Date of Receipt : 14 Jan.2025

Date of Calibration : 24-27 Feb.2025

1 / 9

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FMBL.MTC.002 Rev.5

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9009

Office/Laboratory
668 Mu 2 Tambon Bangpoo, Amphoe Muang Samutprakan,
Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtg@tistr.or.th Website : www.tistr.or.th

Office
196 Phahonyothin Road, Ladysao, Chatuchak,
Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9009

Office/Laboratory
668 Mu 2 Tambon Bangpoo, Amphoe Muang Samutprakan,
Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtg@tistr.or.th Website : www.tistr.or.th

Office
196 Phahonyothin Road, Ladysao, Chatuchak,
Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827



- Power Amplifier Brüel&Kjær 2706 S/N 1517650.
- Speaker Tannoy Limited, Great Britain British Patent No. 215300.
- Digital Multimeter Agilent 34401A S/N MY44005560.
- Programmable Attenuator Tamagawa TPA-303A S/N 2212.

Calibration Procedure :

This instrument was calibrated by using calibration procedures no CP-102-02 and CP-102-03, which were based on IEC 61672-3 Electroacoustics - Sound Level Meters - Part 3 : Periodic tests (2013). These calibration procedures were related to the electrical and acoustic signal tests. The electrical signal test was carried out with the direct measurement method. The acoustic signal test was performed in an anechoic room with the comparison measurement method.

This instrument has been calibrated against standards maintained at the Electrical and Electronic Standards Laboratory (EEL), which are traceable to the International System of Units through the National Institute of Metrology (Thailand).

The information on actual reading is attached herewith and the uncertainty limits quoted refer to the measured values only.

The reported expanded uncertainty is based upon a standard uncertainty multiplied by a coverage factor $k=2$, providing a level of confidence of approximately 95%.

Date of Calibration : 24-27 Feb.2025

2 / 9

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FMBL.MTC.002 Rev.5

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9009

Office/Laboratory
668 Mu 2 Tambon Bangpoo, Amphoe Muang Samutprakan,
Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtg@tistr.or.th Website : www.tistr.or.th

Office
196 Phahonyothin Road, Ladysao, Chatuchak,
Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9009

Office/Laboratory
668 Mu 2 Tambon Bangpoo, Amphoe Muang Samutprakan,
Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtg@tistr.or.th Website : www.tistr.or.th

Office
196 Phahonyothin Road, Ladysao, Chatuchak,
Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827

1. Absolute Sensitivity

Reference Acoustic Signal (dB)	Measured value (dB)	Deviation value (dB)	Acceptance limit Class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
93.99	94.0	0.0	1.0	0.48	N/A

Note: No adjustment.

2. Self-generated noise

2.1 Normal test

Measured value (dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
20.8	0.10	N/A

2.2 The microphone of the sound level meter was replaced by electrical signal input device

Frequency Weighting	Measured value (dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
A-Weight	13.3	0.10	N/A
C-Weight	18.4	0.10	N/A
Flat	22.4	0.10	N/A

Date of Calibration : 24-27 Feb.2025

3 / 9

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FMBL.MTC.002 Rev.5

3. Acoustical signal test of frequency weightings

Frequency (Hz)	Deviation from frequency response (dB)			Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
	A-weight	C-weight	Flat			
125	0.2	0.3	0.2	1.5	0.45	0.6
1 000	0.1	0.1	0.2	1.0	0.45	0.6
8 000	-1.6	-1.5	-1.1	5.0	0.45	0.7

4. Electrical signal test of frequency weightings

Frequency (Hz)	Deviation from frequency response (dB)			Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
	A-weight	C-weight	Flat			
63	0.0	0.0	-0.1	2.0	0.20	0.6
125	0.0	0.0	0.0	1.5	0.20	0.6
250	0.0	0.0	0.0	1.5	0.20	0.6
500	0.0	0.0	0.0	1.5	0.20	0.6
1 000	0.0	0.0	0.0	1.0	0.20	0.6
2 000	-0.1	-0.1	-0.1	2.0	0.20	0.6
4 000	-0.4	-0.4	-0.1	3.0	0.20	0.6
8 000	-0.6	-0.7	-0.2	5.0	0.20	0.7

Date of Calibration : 24-27 Feb.2025

4 / 9

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BLMTC.002 Rev.5

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9039

Office/Laboratory
668 Mu 2 Tambon Bangpookai, Amphoe Muang Samutprakarn,
Changwat Samutprakarn 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtg@tistr.or.th Website : www.tistr.or.th

Office
196 Phahonyothin Road, Ladysao, Chatuchak,
Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827

7. Level linearity on the reference level range

Anticipated value (dB)	Measured Value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
122	122.0	0.0	1.1	0.30	0.3
121	121.1	0.1	1.1	0.30	0.3
120	120.1	0.1	1.1	0.30	0.3
119	119.1	0.1	1.1	0.30	0.3
114	114.0	0.0	1.1	0.30	0.3
109	109.0	0.0	1.1	0.30	0.3
104	104.0	0.0	1.1	0.30	0.3
99	99.0	0.0	1.1	0.30	0.3
94	94.0	0.0	1.1	0.30	0.3
89	89.0	0.0	1.1	0.30	0.3
84	84.0	0.0	1.1	0.30	0.3
79	79.1	0.1	1.1	0.30	0.3
74	74.1	0.1	1.1	0.30	0.3
69	69.1	0.1	1.1	0.30	0.3
64	64.0	0.0	1.1	0.30	0.3
59	59.0	0.0	1.1	0.30	0.3
54	54.0	0.0	1.1	0.30	0.3
49	49.0	0.0	1.1	0.30	0.3
44	44.0	0.0	1.1	0.30	0.3
39	39.0	0.0	1.1	0.30	0.3
34	34.1	0.1	1.1	0.30	0.3
33	33.1	0.1	1.1	0.30	0.3

Date of Calibration : 24-27 Feb.2025

6 / 9

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BLMTC.002 Rev.5

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9039

Office/Laboratory
668 Mu 2 Tambon Bangpookai, Amphoe Muang Samutprakarn,
Changwat Samutprakarn 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtg@tistr.or.th Website : www.tistr.or.th

Office
196 Phahonyothin Road, Ladysao, Chatuchak,
Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827

5. Long-term stability

Time	Measured Value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Begin	94.0	0.0	0.3	0.10	0.1
End	94.0				

6. Frequency and time weightings at 1 kHz

6.1 Frequency weightings at 1 kHz

Frequency Weighting	Measured Value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
A-weight	94.0	0.0	0.2	0.20	0.2
C-weight	94.0	0.0	0.2	0.20	0.2
Flat	94.1	0.1	0.2	0.20	0.2

6.2 Time weightings at 1 kHz

Frequency Weighting	Measured Value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Fast	94.0	0.0	0.1	0.20	0.2
Slow	94.0	0.0	0.1	0.20	0.2
Leq	94.0	0.0	0.1	0.20	0.2

Date of Calibration : 24-27 Feb.2025

5 / 9

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BLMTC.002 Rev.5

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9039

Office/Laboratory
668 Mu 2 Tambon Bangpookai, Amphoe Muang Samutprakarn,
Changwat Samutprakarn 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtg@tistr.or.th Website : www.tistr.or.th

Office
196 Phahonyothin Road, Ladysao, Chatuchak,
Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827

7. Level linearity on the reference level range

Anticipated value (dB)	Measured Value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
32	32.2	0.2	1.1	0.30	0.3
31	31.2	0.2	1.1	0.30	0.3
30	30.3	0.3	1.1	0.30	0.3

8. Level linearity including the level range control

Range	Anticipated value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
40-130	94.0	94.0	0.0	1.1	0.30	0.3
30-120	94.0	94.0	0.0	1.1	0.30	0.3
20-110	94.0	94.0	0.0	1.1	0.30	0.3
20-100	94.0	94.0	0.0	1.1	0.30	0.3

Date of Calibration : 24-27 Feb.2025

7 / 9

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BLMTC.002 Rev.5

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9039

Office/Laboratory
668 Mu 2 Tambon Bangpookai, Amphoe Muang Samutprakarn,
Changwat Samutprakarn 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtg@tistr.or.th Website : www.tistr.or.th

Office
196 Phahonyothin Road, Ladysao, Chatuchak,
Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827

8. Level linearity including the level range control

At reference level at 5 dB greater than the under-range on a level range

Range	Anticipated value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
40-130	45.0	45.0	0.0	1.1	0.30	0.3
30-120	35.0	35.0	0.0	1.1	0.30	0.3
20-110	25.0	25.3	0.3	1.1	0.30	0.3
20-100	25.0	25.2	0.2	1.1	0.30	0.3
20-90	25.0	25.2	0.2	1.1	0.30	0.3
20-80	25.0	25.2	0.2	1.1	0.30	0.3

9. Tone burst response

Time Weighting	Toneburst Duration, T _b (ms)	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Fast	200	115.8	-0.2	±1.0	0.20	0.3
	2	98.3	-0.7	+1.0; -2.5	0.20	0.3
	0.25	89.2	-0.8	+1.5; -5.0	0.20	0.3
Slow	200	109.5	-0.1	±1.0	0.20	0.3
	2	89.7	-0.3	+1.0; -5.0	0.20	0.3
SEL	200	109.9	-0.1	±1.0	0.20	0.3
	2	89.9	-0.1	+1.0; -2.5	0.20	0.3
	0.25	80.9	-0.1	+1.5; -5.0	0.20	0.3

Date of Calibration : 24-27 Feb.2025

8 / 9

The results relate only to the items tested/calibrated or value assigned. Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FMBL.MTC.002 Rev.5

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang, Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9009

Office/Laboratory
668 Mu 2 Tambon Bangpoomai, Amphoe Muang Samutprakan, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtg@tistr.or.th Website : www.tistr.or.th

Office
196 Phahonyothin Road, Ladysao, Chatuchak, Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827

CALIBRATION CERTIFICATE

Submitted by : Integrated Research Center Company Limited.

Address : 122 Moo 2, T.Thatoom, A.Srimahaphote, Prachinburi 25140.

Calibrated at : Electrical and Electronic Standards Laboratory, Industrial Metrology and Testing Service Centre.
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Rd., A.Muang, Samutprakan 10280.

Instrument Calibrated :	Ambient Environment
Description : Sound Level Meter	Temperature : (23 ± 3) °C
Manufacturer : ACO	Relative Humidity : (50 ± 15) %
Model : 6236	Ambient Pressure : (101.325±1.5) kPa
Serial No. : 192015	
Microphone : 7052NR No.73304	
Preamplifier : -	

- Standards used :
1. Band Pass Filter Stanford Research Systems SR 650 S/N 28712.
 2. Condenser Microphone Brüel&Kjær 4180 S/N 2889871.
 3. Decade Attenuator Ando AL-205 S/N 00464602.
 4. Function/Arbitrary Waveform Generator Agilent 33220A S/N MY44042668.
 5. Digital Function Synthesizer NF Electronic Instruments DF-193A S/N 122037.
 6. Sound Calibrator Brüel&Kjær 4231 S/N 3015154.
 7. Measuring Amplifier Brüel&Kjær 2636 S/N 1537484.

Date of Receipt : 14 Jan.2025

Date of Calibration : 24-27 Feb.2025

1 / 9

The results relate only to the items tested/calibrated or value assigned. Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FMBL.MTC.002 Rev.5

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang, Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9009

Office/Laboratory
668 Mu 2 Tambon Bangpoomai, Amphoe Muang Samutprakan, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtg@tistr.or.th Website : www.tistr.or.th

Office
196 Phahonyothin Road, Ladysao, Chatuchak, Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827

10. Peak C sound level

Number of cycles in test signal	Anticipated value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Complete cycle	125.4	125.7	0.3	3.0	0.20	0.35
Positive half cycle	124.4	124.2	-0.2	2.0	0.20	0.35
Negative half cycle	124.4	124.2	-0.2	2.0	0.20	0.35

11. Overload indication

Measured value (dB)		Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Positive one-half cycle	Negative one-half cycle				
132.5	132.5	0.0	1.5	0.20	0.25

12. High-level stability

Time	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Begin	129.0	0.0	0.3	0.10	0.1
End	129.0				

Calibrated by :

Tawikiat Iamsamran
.....
(Mr. Tawikiat Iamsamran)

Approved by :

Prawate Klusaypa
.....
(Mr. Prawate Klusaypa)
Director

Electrical and Electronic Standards Laboratory

Industrial Metrology and Testing Service Centre

Date of Calibration : 24-27 Feb.2025

Date of Issue : 28 Feb.2025

Ref : 2011268011400185003

End of Certificate

9 / 9

The results relate only to the items tested/calibrated or value assigned. Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FMBL.MTC.002 Rev.5

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang, Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9009

Office/Laboratory
668 Mu 2 Tambon Bangpoomai, Amphoe Muang Samutprakan, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtg@tistr.or.th Website : www.tistr.or.th

Office
196 Phahonyothin Road, Ladysao, Chatuchak, Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827

8. Power Amplifier Brüel&Kjær 2706 S/N 1517650.
9. Speaker Tannoy Limited, Great Britain British Patent No. 215300.
10. Digital Multimeter Agilent 34401A S/N MY44005560.
11. Programmable Attenuator Tamagawa TPA-303A S/N 2212.

Calibration Procedure :

This instrument was calibrated by using calibration procedures no CP-102-02 and CP-102-03, which were based on IEC 61672-3 Electroacoustics - Sound Level Meters - Part 3 : Periodic tests (2013). These calibration procedures were related to the electrical and acoustic signal tests. The electrical signal test was carried out with the direct measurement method. The acoustic signal test was performed in an anechoic room with the comparison measurement method.

This instrument has been calibrated against standards maintained at the Electrical and Electronic Standards Laboratory (EEL), which are traceable to the International System of Units through the National Institute of Metrology (Thailand).

The information on actual reading is attached herewith and the uncertainty limits quoted refer to the measured values only.

The reported expanded uncertainty is based upon a standard uncertainty multiplied by a coverage factor k=2, providing a level of confidence of approximately 95%.

Date of Calibration : 24-27 Feb.2025

2 / 9

The results relate only to the items tested/calibrated or value assigned. Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FMBL.MTC.002 Rev.5

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang, Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9009

Office/Laboratory
668 Mu 2 Tambon Bangpoomai, Amphoe Muang Samutprakan, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtg@tistr.or.th Website : www.tistr.or.th

Office
196 Phahonyothin Road, Ladysao, Chatuchak, Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827

1. Absolute Sensitivity

Reference Acoustic Signal (dB)	Measured value (dB)	Deviation value (dB)	Acceptance limit Class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
93.99	93.9	-0.1	1.0	0.48	N/A

Note: No adjustment.

2. Self-generated noise

2.1 Normal test

Measured value (dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
22.0	0.10	N/A

2.2 The microphone of the sound level meter was replaced by electrical signal input device

Frequency Weighting	Measured value (dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
A-Weight	15.7	0.10	N/A
C-Weight	21.5	0.10	N/A
Flat	26.0	0.10	N/A

Date of Calibration : 24-27 Feb.2025

3 / 9

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FMBL/MTC.002 Rev.5

3. Acoustical signal test of frequency weightings

Frequency (Hz)	Deviation from frequency response (dB)			Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
	A-weight	C-weight	Flat			
125	0.4	0.4	0.4	1.5	0.45	0.6
1 000	-0.4	-0.4	-0.4	1.0	0.45	0.6
8 000	-0.8	-1.0	-0.6	5.0	0.45	0.7

4. Electrical signal test of frequency weightings

Frequency (Hz)	Deviation from frequency response (dB)			Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
	A-weight	C-weight	Flat			
63	0.1	0.0	-0.1	2.0	0.20	0.6
125	0.0	0.0	0.0	1.5	0.20	0.6
250	0.0	0.0	0.0	1.5	0.20	0.6
500	0.0	0.0	0.0	1.5	0.20	0.6
1 000	0.0	0.0	0.0	1.0	0.20	0.6
2 000	-0.1	0.0	-0.1	2.0	0.20	0.6
4 000	-0.4	-0.4	-0.1	3.0	0.20	0.6
8 000	-0.6	-0.6	-0.2	5.0	0.20	0.7

Date of Calibration : 24-27 Feb.2025

4 / 9

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FMBL/MTC.002 Rev.5

5. Long-term stability

Time	Measured Value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Begin	94.0	0.0	0.3	0.10	0.1
End	94.0				

6. Frequency and time weightings at 1 kHz

6.1 Frequency weightings at 1 kHz

Frequency Weighting	Measured Value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
A-weight	94.0	0.0	0.2	0.20	0.2
C-weight	94.0	0.0	0.2	0.20	0.2
Flat	94.0	0.0	0.2	0.20	0.2

6.2 Time weightings at 1 kHz

Frequency Weighting	Measured Value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Fast	94.0	0.0	0.1	0.20	0.2
Slow	94.0	0.0	0.1	0.20	0.2
Leq	94.0	0.0	0.1	0.20	0.2

Date of Calibration : 24-27 Feb.2025

5 / 9

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FMBL/MTC.002 Rev.5

7. Level linearity on the reference level range

Anticipated value (dB)	Measured Value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
122	122.1	0.1	1.1	0.30	0.3
121	121.1	0.1	1.1	0.30	0.3
120	120.1	0.1	1.1	0.30	0.3
119	119.1	0.1	1.1	0.30	0.3
114	114.0	0.0	1.1	0.30	0.3
109	109.0	0.0	1.1	0.30	0.3
104	104.0	0.0	1.1	0.30	0.3
99	99.0	0.0	1.1	0.30	0.3
94	94.0	0.0	1.1	0.30	0.3
89	89.0	0.0	1.1	0.30	0.3
84	84.0	0.0	1.1	0.30	0.3
79	79.1	0.1	1.1	0.30	0.3
74	74.2	0.2	1.1	0.30	0.3
69	69.2	0.2	1.1	0.30	0.3
64	64.0	0.0	1.1	0.30	0.3
59	59.1	0.1	1.1	0.30	0.3
54	54.1	0.1	1.1	0.30	0.3
49	49.1	0.1	1.1	0.30	0.3
44	44.1	0.1	1.1	0.30	0.3
39	39.1	0.1	1.1	0.30	0.3
34	34.2	0.2	1.1	0.30	0.3
33	33.3	0.3	1.1	0.30	0.3

Date of Calibration : 24-27 Feb.2025

6 / 9

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FMBL/MTC.002 Rev.5

7. Level linearity on the reference level range

Anticipated value (dB)	Measured Value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
32	32.3	0.3	1.1	0.30	0.3
31	31.4	0.4	1.1	0.30	0.3
30	30.4	0.4	1.1	0.30	0.3

8. Level linearity including the level range control

At reference sound level on the reference level range

Range	Anticipated value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
40-130	94.0	94.0	0.0	1.1	0.30	0.3
30-120	94.0	94.0	0.0	1.1	0.30	0.3
20-110	94.0	94.0	0.0	1.1	0.30	0.3
20-100	94.0	94.0	0.0	1.1	0.30	0.3

Date of Calibration : 24-27 Feb.2025

7 / 9

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FMBL/MTC.002 Rev.5

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang, Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9009

Office/Laboratory
668 Mu 2 Tambon Bangpoornai, Amphoe Muang Samutprakan, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtc@tistr.or.th Website : www.tistr.or.th

Office
196 Phahonyothin Road, Ladysao, Chatuchak, Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827

10. Peak C sound level

Number of cycles in test signal	Anticipated value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Complete cycle	125.4	125.5	0.1	3.0	0.20	0.35
Positive half cycle	124.4	124.3	-0.1	2.0	0.20	0.35
Negative half cycle	124.4	124.3	-0.1	2.0	0.20	0.35

11. Overload indication

Measured value (dB)		Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Positive one-half cycle	Negative one-half cycle	0.0	1.5	0.20	0.25
132.5	132.5				

12. High-level stability

Time	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Begin	129.0	0.0	0.3	0.10	0.1
End	129.0				

Calibrated by :
(Signature)
(Mr. Tawikiat Iamsamran)

Approved by :
(Signature)
(Mr. Prawate Klaiyapa)
Director

Electrical and Electronic Standards Laboratory
Industrial Metrology and Testing Service Centre

Date of Calibration : 24-27 Feb.2025

Date of Issue : 28 Feb.2025

Ref : 2011268011400185002

End of Certificate

9 / 9

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FMBL/MTC.002 Rev.5

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang, Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9009

Office/Laboratory
668 Mu 2 Tambon Bangpoornai, Amphoe Muang Samutprakan, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtc@tistr.or.th Website : www.tistr.or.th

Office
196 Phahonyothin Road, Ladysao, Chatuchak, Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827

8. Level linearity including the level range control

At reference level at 5 dB greater than the under-range on a level range

Range	Anticipated value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
40-130	45.0	45.0	0.0	1.1	0.30	0.3
30-120	35.0	35.0	0.0	1.1	0.30	0.3
20-110	25.0	25.5	0.5	1.1	0.30	0.3
20-100	25.0	25.4	0.4	1.1	0.30	0.3
20-90	25.0	25.4	0.4	1.1	0.30	0.3
20-80	25.0	25.2	0.2	1.1	0.30	0.3

9. Tone burst response

Time Weighting	Toneburst Duration, Tb (ms)	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Fast	200	115.8	-0.2	±1.0	0.20	0.3
	2	98.6	-0.4	+1.0; -2.5	0.20	0.3
	0.25	89.0	-1.0	+1.5; -5.0	0.20	0.3
Slow	200	109.4	-0.2	±1.0	0.20	0.3
	2	89.8	-0.2	+1.0; -5.0	0.20	0.3
	0.25	80.9	-1.0	+1.5; -5.0	0.20	0.3
SEL	200	109.9	-0.1	±1.0	0.20	0.3
	2	90.0	0.0	+1.0; -2.5	0.20	0.3
	0.25	80.9	-0.1	+1.5; -5.0	0.20	0.3

Date of Calibration : 24-27 Feb.2025

8 / 9

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FMBL/MTC.002 Rev.5

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang, Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9009

Office/Laboratory
668 Mu 2 Tambon Bangpoornai, Amphoe Muang Samutprakan, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtc@tistr.or.th Website : www.tistr.or.th

Office
196 Phahonyothin Road, Ladysao, Chatuchak, Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827

CALIBRATION CERTIFICATE

Submitted by : Integrated Research Center Company Limited.

Address : 122 Moo 2, T.Thatoom, A.Srimahaphote, Prachinburi 25140.

Calibrated at : Electrical and Electronic Standards Laboratory, Industrial Metrology and Testing Service Centre.
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Rd., A.Muang, Samutprakan 10280.

Instrument Calibrated :

Description : Sound Level Meter
Manufacturer : ACO
Model : 6236
Serial No. : 192016
Microphone : 7052NR No.73305
Pre-amplifier :-

Ambient Environment

Temperature : (23 ± 3) °C
Relative Humidity : (50 ± 15) %
Ambient Pressure : (101.325±1.5) kPa

Standards used :

- Band Pass Filter Stanford Research Systems SR 650 S/N 28712.
- Condenser Microphone Brüel&Kjær 4180 S/N 2889871.
- Decade Attenuator Ando AL-205 S/N 00464602.
- Function/Arbitrary Waveform Generator Agilent 33220A S/N MY44042668.
- Digital Function Synthesizer NF Electronic Instruments DF-193A S/N 122037.
- Sound Calibrator Brüel&Kjær 4231 S/N 3015154.
- Measuring Amplifier Brüel&Kjær 2636 S/N 1537484.

Date of Receipt : 14 Jan.2025

Date of Calibration : 24-27 Feb.2025

1 / 9

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FMBL/MTC.002 Rev.5

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang, Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9009

Office/Laboratory
668 Mu 2 Tambon Bangpoornai, Amphoe Muang Samutprakan, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtc@tistr.or.th Website : www.tistr.or.th

Office
196 Phahonyothin Road, Ladysao, Chatuchak, Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827

8. Power Amplifier Brüel&Kjær 2706 S/N 1517650.
9. Speaker Tannoy Limited, Great Britain British Patent No. 215300.
10. Digital Multimeter Agilent 34401A S/N MY44005560.
11. Programmable Attenuator Tamagawa TPA-303A S/N 2212.

Calibration Procedure :

This instrument was calibrated by using calibration procedures no CP-102-02 and CP-102-03, which were based on IEC 61672-3 Electroacoustics - Sound Level Meters - Part 3 : Periodic tests (2013). These calibration procedures were related to the electrical and acoustic signal tests. The electrical signal test was carried out with the direct measurement method. The acoustic signal test was performed in an anechoic room with the comparison measurement method.

This instrument has been calibrated against standards maintained at the Electrical and Electronic Standards Laboratory (EEL), which are traceable to the International System of Units through the National Institute of Metrology (Thailand).

The information on actual reading is attached herewith and the uncertainty limits quoted refer to the measured values only.

The reported expanded uncertainty is based upon a standard uncertainty multiplied by a coverage factor $k=2$, providing a level of confidence of approximately 95%.

Date of Calibration : 24-27 Feb.2025

 2 / 9
 et

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

1. Absolute Sensitivity

Reference Acoustic Signal (dB)	Measured value (dB)	Deviation value (dB)	Acceptance limit Class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
93.99	93.3	-0.7	1.0	0.48	N/A

Note: No adjustment.

2. Self-generated noise
2.1 Normal test

Measured value (dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
23.6	0.10	N/A

2.2 The microphone of the sound level meter was replaced by electrical signal input device

Frequency Weighting	Measured value (dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
A-Weight	15.5	0.10	N/A
C-Weight	20.5	0.10	N/A
Flat	25.1	0.10	N/A

Date of Calibration : 24-27 Feb.2025

 3 / 9
 et

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

3. Acoustical signal test of frequency weightings

Frequency (Hz)	Deviation from frequency response (dB)			Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
	A-weight	C-weight	Flat			
125	0.5	0.6	0.5	1.5	0.45	0.6
1 000	-0.9	-0.9	-0.8	1.0	0.45	0.6
8 000	-1.3	-1.1	-0.7	5.0	0.45	0.7

4. Electrical signal test of frequency weightings

Frequency (Hz)	Deviation from frequency response (dB)			Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
	A-weight	C-weight	Flat			
63	0.1	0.0	-0.1	2.0	0.20	0.6
125	0.0	0.0	0.0	1.5	0.20	0.6
250	0.0	0.0	0.0	1.5	0.20	0.6
500	0.0	0.0	0.0	1.5	0.20	0.6
1 000	0.0	0.0	0.0	1.0	0.20	0.6
2 000	-0.1	-0.1	0.0	2.0	0.20	0.6
4 000	-0.4	-0.4	-0.1	3.0	0.20	0.6
8 000	-0.7	-0.6	-0.2	5.0	0.20	0.7

Date of Calibration : 24-27 Feb.2025

 4 / 9
 et

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

5. Long-term stability

Time	Measured Value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Begin	94.0	0.0	0.3	0.10	0.1
End	94.0				

6. Frequency and time weightings at 1 kHz
6.1 Frequency weightings at 1 kHz

Frequency Weighting	Measured Value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
A-weight	94.0	0.0	0.2	0.20	0.2
C-weight	94.0	0.0	0.2	0.20	0.2
Flat	94.1	0.1	0.2	0.20	0.2

6.2 Time weightings at 1 kHz

Frequency Weighting	Measured Value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Fast	94.0	0.0	0.1	0.20	0.2
Slow	94.0	0.0	0.1	0.20	0.2
Leq	94.0	0.0	0.1	0.20	0.2

Date of Calibration : 24-27 Feb.2025

 5 / 9
 et

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

7. Level linearity on the reference level range

Anticipated value (dB)	Measured Value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
122	121.9	-0.1	1.1	0.30	0.3
121	120.9	-0.1	1.1	0.30	0.3
120	119.9	-0.1	1.1	0.30	0.3
119	118.9	-0.1	1.1	0.30	0.3
114	113.9	-0.1	1.1	0.30	0.3
109	109.0	0.0	1.1	0.30	0.3
104	104.0	0.0	1.1	0.30	0.3
99	99.0	0.0	1.1	0.30	0.3
94	94.0	0.0	1.1	0.30	0.3
89	89.0	0.0	1.1	0.30	0.3
84	84.1	0.1	1.1	0.30	0.3
79	79.1	0.1	1.1	0.30	0.3
74	74.1	0.1	1.1	0.30	0.3
69	69.2	0.2	1.1	0.30	0.3
64	64.0	0.0	1.1	0.30	0.3
59	59.1	0.1	1.1	0.30	0.3
54	54.0	0.0	1.1	0.30	0.3
49	49.1	0.1	1.1	0.30	0.3
44	44.1	0.1	1.1	0.30	0.3
39	39.1	0.1	1.1	0.30	0.3
34	34.2	0.2	1.1	0.30	0.3
33	33.3	0.3	1.1	0.30	0.3

Date of Calibration : 24-27 Feb.2025

6/9

The results relate only to the items tested/calibrated or value assigned. Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang, Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9009

Office/Laboratory
668 Mu 2 Tambon Bangpoornai, Amphoe Muang Samutprakarn, Changwat Samutprakarn 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtg@tistr.or.th Website : www.tistr.or.th

Office
196 Phahonyothin Road, Laddoo, Chatuchak, Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827

FMBL/MTC.002 Rev.5

8. Level linearity including the level range control

At reference level at 5 dB greater than the under-range on a level range

Range	Anticipated value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
40-130	45.0	44.9	-0.1	1.1	0.30	0.3
30-120	35.0	35.0	0.0	1.1	0.30	0.3
20-110	25.0	25.7	0.7	1.1	0.30	0.3
20-100	25.0	25.6	0.6	1.1	0.30	0.3
20-90	25.0	25.5	0.5	1.1	0.30	0.3
20-80	25.0	25.4	0.4	1.1	0.30	0.3

9. Tone burst response

Time Weighting	Toneburst Duration, Tb (ms)	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Fast	200	116.0	0.0	±1.0	0.20	0.3
	2	98.6	-0.4	+1.0; -2.5	0.20	0.3
	0.25	89.5	-0.5	+1.5; -5.0	0.20	0.3
Slow	200	109.5	-0.1	±1.0	0.20	0.3
	2	89.8	-0.2	+1.0; -5.0	0.20	0.3
	200	109.9	-0.1	±1.0	0.20	0.3
SEL	2	89.9	-0.1	+1.0; -2.5	0.20	0.3
	0.25	80.9	-0.1	+1.5; -5.0	0.20	0.3

Date of Calibration : 24-27 Feb.2025

8/9

The results relate only to the items tested/calibrated or value assigned. Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang, Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9009

Office/Laboratory
668 Mu 2 Tambon Bangpoornai, Amphoe Muang Samutprakarn, Changwat Samutprakarn 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtg@tistr.or.th Website : www.tistr.or.th

Office
196 Phahonyothin Road, Laddoo, Chatuchak, Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827

FMBL/MTC.002 Rev.5

7. Level linearity on the reference level range

Anticipated value (dB)	Measured Value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
32	32.4	0.4	1.1	0.30	0.3
31	31.5	0.5	1.1	0.30	0.3
30	30.6	0.6	1.1	0.30	0.3

8. Level linearity including the level range control

At reference sound level on the reference level range

Range	Anticipated value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
40-130	94.0	94.0	0.0	1.1	0.30	0.3
30-120	94.0	94.0	0.0	1.1	0.30	0.3
20-110	94.0	94.0	0.0	1.1	0.30	0.3
20-100	94.0	94.0	0.0	1.1	0.30	0.3

Date of Calibration : 24-27 Feb.2025

7/9

The results relate only to the items tested/calibrated or value assigned. Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang, Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9009

Office/Laboratory
668 Mu 2 Tambon Bangpoornai, Amphoe Muang Samutprakarn, Changwat Samutprakarn 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtg@tistr.or.th Website : www.tistr.or.th

Office
196 Phahonyothin Road, Laddoo, Chatuchak, Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827

FMBL/MTC.002 Rev.5

10. Peak C sound level

Number of cycles in test signal	Anticipated value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Complete cycle	125.4	125.1	-0.3	3.0	0.20	0.35
Positive half cycle	124.4	122.4	-2.0	2.0	0.20	0.35
Negative half cycle	124.4	124.6	0.2	2.0	0.20	0.35

11. Overload indication

Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Positive one-half cycle	Negative one-half cycle	0.0	1.5	0.20
132.5	132.5			0.25

12. High-level stability

Time	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Begin	129.0	0.0	0.3	0.10	0.1
End	129.0				

Calibrated by :

(Mr. Tawikiat Iamsamran)

Approved by :

(Mr. Prasart Klusaypa)
Director
Electrical and Electronic Standards Laboratory

Date of Calibration : 24-27 Feb.2025

Date of Issue : 28 Feb.2025

Industrial Metrology and Testing Service Centre

Ref : 2011268011400185001

End of Certificate

9/9

The results relate only to the items tested/calibrated or value assigned. Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang, Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9009

Office/Laboratory
668 Mu 2 Tambon Bangpoornai, Amphoe Muang Samutprakarn, Changwat Samutprakarn 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtg@tistr.or.th Website : www.tistr.or.th

Office
196 Phahonyothin Road, Laddoo, Chatuchak, Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827

FMBL/MTC.002 Rev.5

CALIBRATION CERTIFICATE
Submitted by : Integrated Research Center Company Limited.

Address : 122 Moo 2, T.Thatoom, A.Srimahaphote, Prachinburi 25140.

Calibrated at : Electrical and Electronic Standards Laboratory, Industrial Metrology and Testing Service Centre.
 Soi 1C, Bangpoo Industrial Estate, Sukhumvit Rd., A.Muang, Samutprakan 10280.

Instrument Calibrated :
Description : Sound Level Meter
Manufacturer : ACO
Model : 6236
Serial No. : 212014
Microphone : 7052NR No.76235
Preamplifier : -

Ambient Environment
Temperature : (23 ± 3) °C
Relative Humidity : (50 ± 15) %
Ambient Pressure : (101.325±1.5) kPa

Standards used :

1. Band Pass Filter Stanford Research Systems SR 650 S/N 28712.
2. Condenser Microphone Brüel&Kjær 4180 S/N 2889871.
3. Decade Attenuator Ando AL-205 S/N 00464602.
4. Function/Arbitrary Waveform Generator Agilent 33220A S/N MY44042668.
5. Digital Function Synthesizer NF Electronic Instruments DF-193A S/N 122037.
6. Sound Calibrator Brüel&Kjær 4231 S/N 3015154.
7. Measuring Amplifier Brüel&Kjær 2636 S/N 1537484.

Date of Receipt : 14 Jan.2025

Date of Calibration : 24-27 Feb.2025

1 / 9

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FMBL.MTC.002 Rev.5

Head Office
 35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
 Changwat Pathumthani 12120, Thailand
 Tel. (66) 0 2577 9036
 Fax. (66) 0 2577 9009

Office/Laboratory
 668 Mu 2 Tambon Bangpooam, Amphoe Muang Samutprakan,
 Changwat Samutprakan 10280, Thailand
 Tel. (66) 0 2323 1672-80 ext. 115, 116
 (66) 08 3219 9440
 E-mail : mtctr@tistr.or.th Website : www.tistr.or.th

Office
 196 Phahonyothin Road, Ladysao, Chatuchak,
 Bangkok 10900, Thailand
 Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
 (66) 08 1889 6827

1. Absolute Sensitivity

Reference Acoustic Signal (dB)	Measured value (dB)		Deviation value (dB)	Acceptance limit Class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
	Before adjust	After adjust				
93.99	94.2	94.0	0.0	1.0	0.48	N/A

Note: The external calibration adjustment was firstly performed. The internal calibration adjustment was then completed at the display of 114.7 dB.

2. Self-generated noise
2.1 Normal test

Measured value (dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
20.7	0.10	N/A

2.2 The microphone of the sound level meter was replaced by electrical signal input device

Frequency Weighting	Measured value (dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
A-Weight	13.7	0.10	N/A
C-Weight	19.0	0.10	N/A
Flat	23.9	0.10	N/A

Date of Calibration : 24-27 Feb.2025

3 / 9

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FMBL.MTC.002 Rev.5

Head Office
 35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
 Changwat Pathumthani 12120, Thailand
 Tel. (66) 0 2577 9036
 Fax. (66) 0 2577 9009

Office/Laboratory
 668 Mu 2 Tambon Bangpooam, Amphoe Muang Samutprakan,
 Changwat Samutprakan 10280, Thailand
 Tel. (66) 0 2323 1672-80 ext. 115, 116
 (66) 08 3219 9440
 E-mail : mtctr@tistr.or.th Website : www.tistr.or.th

Office
 196 Phahonyothin Road, Ladysao, Chatuchak,
 Bangkok 10900, Thailand
 Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
 (66) 08 1889 6827

8. Power Amplifier Brüel&Kjær 2706 S/N 1517650.
9. Speaker Tannoy Limited, Great Britain British Patent No. 215300.
10. Digital Multimeter Agilent 34401A S/N MY44005560.
11. Programmable Attenuator Tamagawa TPA-303A S/N 2212.

Calibration Procedure :

This instrument was calibrated by using calibration procedures no CP-102-02 and CP-102-03, which were based on IEC 61672-3 Electroacoustics - Sound Level Meters - Part 3 : Periodic tests (2013). These calibration procedures were related to the electrical and acoustic signal tests. The electrical signal test was carried out with the direct measurement method. The acoustic signal test was performed in an anechoic room with the comparison measurement method.

This instrument has been calibrated against standards maintained at the Electrical and Electronic Standards Laboratory (EEL), which are traceable to the International System of Units through the National Institute of Metrology (Thailand).

The information on actual reading is attached herewith and the uncertainty limits quoted refer to the measured values only.

The reported expanded uncertainty is based upon a standard uncertainty multiplied by a coverage factor k=2, providing a level of confidence of approximately 95%.

Date of Calibration : 24-27 Feb.2025

2 / 9

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FMBL.MTC.002 Rev.5

Head Office
 35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
 Changwat Pathumthani 12120, Thailand
 Tel. (66) 0 2577 9036
 Fax. (66) 0 2577 9009

Office/Laboratory
 668 Mu 2 Tambon Bangpooam, Amphoe Muang Samutprakan,
 Changwat Samutprakan 10280, Thailand
 Tel. (66) 0 2323 1672-80 ext. 115, 116
 (66) 08 3219 9440
 E-mail : mtctr@tistr.or.th Website : www.tistr.or.th

Office
 196 Phahonyothin Road, Ladysao, Chatuchak,
 Bangkok 10900, Thailand
 Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
 (66) 08 1889 6827

3. Acoustical signal test of frequency weightings

Frequency (Hz)	Deviation from frequency response (dB)			Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
	A-weight	C-weight	Flat			
125	0.5	0.5	0.3	1.5	0.45	0.6
1 000	-0.1	-0.2	0.0	1.0	0.45	0.6
8 000	-1.3	-1.1	-0.8	5.0	0.45	0.7

4. Electrical signal test of frequency weightings

Frequency (Hz)	Deviation from frequency response (dB)			Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
	A-weight	C-weight	Flat			
63	0.2	0.0	-0.1	2.0	0.20	0.6
125	0.1	0.0	0.0	1.5	0.20	0.6
250	0.1	0.0	0.0	1.5	0.20	0.6
500	0.0	0.0	0.0	1.5	0.20	0.6
1 000	0.0	0.0	0.0	1.0	0.20	0.6
2 000	-0.1	0.0	-0.1	2.0	0.20	0.6
4 000	-0.4	-0.3	-0.1	3.0	0.20	0.6
8 000	-0.6	-0.6	-0.2	5.0	0.20	0.7

Date of Calibration : 24-27 Feb.2025

4 / 9

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FMBL.MTC.002 Rev.5

Head Office
 35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
 Changwat Pathumthani 12120, Thailand
 Tel. (66) 0 2577 9036
 Fax. (66) 0 2577 9009

Office/Laboratory
 668 Mu 2 Tambon Bangpooam, Amphoe Muang Samutprakan,
 Changwat Samutprakan 10280, Thailand
 Tel. (66) 0 2323 1672-80 ext. 115, 116
 (66) 08 3219 9440
 E-mail : mtctr@tistr.or.th Website : www.tistr.or.th

Office
 196 Phahonyothin Road, Ladysao, Chatuchak,
 Bangkok 10900, Thailand
 Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
 (66) 08 1889 6827

5. Long-term stability

Time	Measured Value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Begin	94.0	0.0	0.3	0.10	0.1
End	94.0				

6. Frequency and time weightings at 1 kHz

6.1 Frequency weightings at 1 kHz

Frequency Weighting	Measured Value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
A-weight	94.0	0.0	0.2	0.20	0.2
C-weight	94.0	0.0	0.2	0.20	0.2
Flat	94.0	0.0	0.2	0.20	0.2

6.2 Time weightings at 1 kHz

Frequency Weighting	Measured Value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Fast	94.0	0.0	0.1	0.20	0.2
Slow	94.0	0.0	0.1	0.20	0.2
Leq	94.0	0.0	0.1	0.20	0.2

Date of Calibration : 24-27 Feb.2025

5 / 9

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FMBL/MTC.002 Rev.5

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9056
Fax. (66) 0 2577 9009

Office/Laboratory
668 Mu 2 Tambon Bangpoornai, Amphoe Muang Samutprakarn,
Changwat Samutprakarn 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtctr@tistr.or.th Website : www.tistr.or.th

Office
196 Phahonyothin Road, Ladysao, Chatuchak,
Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827

7. Level linearity on the reference level range

Anticipated value (dB)	Measured Value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
32	32.2	0.2	1.1	0.30	0.3
31	31.3	0.3	1.1	0.30	0.3
30	30.3	0.3	1.1	0.30	0.3

8. Level linearity including the level range control

At reference sound level on the reference level range

Range	Anticipated value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
40-130	94.0	94.0	0.0	1.1	0.30	0.3
30-120	94.0	94.0	0.0	1.1	0.30	0.3
20-110	94.0	94.0	0.0	1.1	0.30	0.3
20-100	94.0	94.0	0.0	1.1	0.30	0.3

Date of Calibration : 24-27 Feb.2025

7 / 9

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FMBL/MTC.002 Rev.5

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9056
Fax. (66) 0 2577 9009

Office/Laboratory
668 Mu 2 Tambon Bangpoornai, Amphoe Muang Samutprakarn,
Changwat Samutprakarn 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtctr@tistr.or.th Website : www.tistr.or.th

Office
196 Phahonyothin Road, Ladysao, Chatuchak,
Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827

7. Level linearity on the reference level range

Anticipated value (dB)	Measured Value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
122	122.1	0.1	1.1	0.30	0.3
121	121.1	0.1	1.1	0.30	0.3
120	120.1	0.1	1.1	0.30	0.3
119	119.1	0.1	1.1	0.30	0.3
114	114.0	0.0	1.1	0.30	0.3
109	109.0	0.0	1.1	0.30	0.3
104	104.0	0.0	1.1	0.30	0.3
99	99.0	0.0	1.1	0.30	0.3
94	94.0	0.0	1.1	0.30	0.3
89	89.0	0.0	1.1	0.30	0.3
84	84.0	0.0	1.1	0.30	0.3
79	79.0	0.0	1.1	0.30	0.3
74	74.1	0.1	1.1	0.30	0.3
69	69.1	0.1	1.1	0.30	0.3
64	64.0	0.0	1.1	0.30	0.3
59	59.0	0.0	1.1	0.30	0.3
54	54.0	0.0	1.1	0.30	0.3
49	49.0	0.0	1.1	0.30	0.3
44	44.0	0.0	1.1	0.30	0.3
39	39.0	0.0	1.1	0.30	0.3
34	34.1	0.1	1.1	0.30	0.3
33	33.2	0.2	1.1	0.30	0.3

Date of Calibration : 24-27 Feb.2025

6 / 9

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FMBL/MTC.002 Rev.5

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9056
Fax. (66) 0 2577 9009

Office/Laboratory
668 Mu 2 Tambon Bangpoornai, Amphoe Muang Samutprakarn,
Changwat Samutprakarn 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtctr@tistr.or.th Website : www.tistr.or.th

Office
196 Phahonyothin Road, Ladysao, Chatuchak,
Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827

8. Level linearity including the level range control

At reference level at 5 dB greater than the under-range on a level range

Range	Anticipated value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
40-130	45.0	45.0	0.0	1.1	0.30	0.3
30-120	35.0	35.0	0.0	1.1	0.30	0.3
20-110	25.0	25.3	0.3	1.1	0.30	0.3
20-100	25.0	25.3	0.3	1.1	0.30	0.3
20-90	25.0	25.2	0.2	1.1	0.30	0.3
20-80	25.0	25.2	0.2	1.1	0.30	0.3

9. Tone burst response

Time Weighting	Toneburst Duration, Tb (ms)	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Fast	200	115.8	-0.2	±1.0	0.20	0.3
	2	98.7	-0.3	+1.0; -2.5	0.20	0.3
	0.25	89.2	-0.8	+1.5; -5.0	0.20	0.3
Slow	200	109.5	-0.1	±1.0	0.20	0.3
	2	89.8	-0.2	+1.0; -5.0	0.20	0.3
	200	109.9	-0.1	±1.0	0.20	0.3
SEL	2	89.9	-0.1	+1.0; -2.5	0.20	0.3
	0.25	80.9	-0.1	+1.5; -5.0	0.20	0.3

Date of Calibration : 24-27 Feb.2025

8 / 9

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FMBL/MTC.002 Rev.5

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9056
Fax. (66) 0 2577 9009

Office/Laboratory
668 Mu 2 Tambon Bangpoornai, Amphoe Muang Samutprakarn,
Changwat Samutprakarn 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtctr@tistr.or.th Website : www.tistr.or.th

Office
196 Phahonyothin Road, Ladysao, Chatuchak,
Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827

10. Peak C sound level

Number of cycles in test signal	Anticipated value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Complete cycle	125.4	125.0	-0.4	3.0	0.20	0.35
Positive half cycle	124.4	124.3	-0.1	2.0	0.20	0.35
Negative half cycle	124.4	124.3	-0.1	2.0	0.20	0.35

11. Overload indication

Measured value (dB)		Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Positive one-half cycle	Negative one-half cycle				
132.5	132.5	0.0	1.5	0.20	0.25

12. High-level stability

Time	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Begin	129.0				
End	129.0	0.0	0.3	0.10	0.1

Calibrated by :

Approved by :

(Mr. Tawikiat Iamsamran)

(Mr. Prawate Khuyapa)

Electrical and Electronic Standards Laboratory
Industrial Metrology and Testing Service Centre

Date of Calibration : 24-27 Feb.2025

Date of Issue : 28 Feb.2025

Ref : 2011268011400185004

End of Certificate

9 / 9

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FMBL.MTC.002 Rev.5

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9039

Office/Laboratory
668 Mu 2 Tambon Bangpoornai, Amphoe Muang Samutprakan,
Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9400
E-mail : mtctr@tistr.or.th Website : www.tistr.or.th

Office
196 Phahonyothin Road, Ladysao, Chatuchak,
Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827

- Power Amplifier Brüel&Kjær 2706 S/N 1517650.
- Speaker Tannoy Limited, Great Britain British Patent No. 215300.
- Digital Multimeter Agilent 34401A S/N MY44005560.
- Programmable Attenuator Tamagawa TPA-303A S/N 2212.

Calibration Procedure :

This instrument was calibrated by using calibration procedures no CP-102-02 and CP-102-03, which were based on IEC 61672-3 Electroacoustics - Sound Level Meters - Part 3 : Periodic tests (2013). These calibration procedures were related to the electrical and acoustic signal tests. The electrical signal test was carried out with the direct measurement method. The acoustic signal test was performed in an anechoic room with the comparison measurement method.

This instrument has been calibrated against standards maintained at the Electrical and Electronic Standards Laboratory (EEL), which are traceable to the International System of Units through the National Institute of Metrology (Thailand).

The information on actual reading is attached herewith and the uncertainty limits quoted refer to the measured values only.

The reported expanded uncertainty is based upon a standard uncertainty multiplied by a coverage factor $k=2$, providing a level of confidence of approximately 95%.

Date of Calibration : 24-27 Feb.2025

2 / 9

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FMBL.MTC.002 Rev.5

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9039

Office/Laboratory
668 Mu 2 Tambon Bangpoornai, Amphoe Muang Samutprakan,
Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9400
E-mail : mtctr@tistr.or.th Website : www.tistr.or.th

Office
196 Phahonyothin Road, Ladysao, Chatuchak,
Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827

CALIBRATION CERTIFICATE

Submitted by : Integrated Research Center Company Limited.

Address : 122 Moo 2, T.Thatoom, A.Srimahaphote, Prachinburi 25140.

Calibrated at : Electrical and Electronic Standards Laboratory, Industrial Metrology and Testing Service Centre.
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Rd., A.Muang, Samutprakan 10280.

Instrument Calibrated :

Ambient Environment

Description : Sound Level Meter

Temperature : (23 ± 3) °C

Manufacturer : ACO

Relative Humidity : (50 ± 15) %

Model : 6236

Ambient Pressure : (101.325±1.5) kPa

Serial No. : 212015

Microphone : 7052NR No.76236

Preamplifier : -

Standards used :

- Band Pass Filter Stanford Research Systems SR 650 S/N 28712.
- Condenser Microphone Brüel&Kjær 4180 S/N 2889871.
- Decade Attenuator Ando AL-205 S/N 00464602.
- Function/Arbitrary Waveform Generator Agilent 33220A S/N MY44042668.
- Digital Function Synthesizer NF Electronic Instruments DF-193A S/N 122037.
- Sound Calibrator Brüel&Kjær 4231 S/N 3015154.
- Measuring Amplifier Brüel&Kjær 2636 S/N 1537484.

Date of Receipt : 14 Jan.2025

Date of Calibration : 24-27 Feb.2025

1 / 9

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FMBL.MTC.002 Rev.5

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9039

Office/Laboratory
668 Mu 2 Tambon Bangpoornai, Amphoe Muang Samutprakan,
Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9400
E-mail : mtctr@tistr.or.th Website : www.tistr.or.th

Office
196 Phahonyothin Road, Ladysao, Chatuchak,
Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827

1. Absolute Sensitivity

Reference Acoustic Signal (dB)	Measured value (dB)		Deviation value (dB)	Acceptance limit Class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
	Before adjust	After adjust				
93.99	94.4	94.0	0.0	1.0	0.48	N/A

Note: The external calibration adjustment was firstly performed. The internal calibration adjustment was then completed at the display of 115.0 dB.

2. Self-generated noise

2.1 Normal test

Measured value (dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
20.7	0.10	N/A

2.2 The microphone of the sound level meter was replaced by electrical signal input device

Frequency Weighting	Measured value (dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
A-Weight	15.1	0.10	N/A
C-Weight	19.9	0.10	N/A
Flat	24.7	0.10	N/A

Date of Calibration : 24-27 Feb.2025

3 / 9

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FMBL.MTC.002 Rev.5

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9039

Office/Laboratory
668 Mu 2 Tambon Bangpoornai, Amphoe Muang Samutprakan,
Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9400
E-mail : mtctr@tistr.or.th Website : www.tistr.or.th

Office
196 Phahonyothin Road, Ladysao, Chatuchak,
Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827

3. Acoustical signal test of frequency weightings

Frequency (Hz)	Deviation from frequency response (dB)			Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
	A-weight	C-weight	Flat			
125	0.4	0.6	0.4	1.5	0.45	0.6
1 000	-0.1	-0.1	0.1	1.0	0.45	0.6
8 000	-0.7	-0.7	-0.2	5.0	0.45	0.7

4. Electrical signal test of frequency weightings

Frequency (Hz)	Deviation from frequency response (dB)			Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
	A-weight	C-weight	Flat			
63	0.0	0.0	-0.1	2.0	0.20	0.6
125	-0.1	0.0	0.0	1.5	0.20	0.6
250	0.0	0.0	0.0	1.5	0.20	0.6
500	0.0	0.0	0.0	1.5	0.20	0.6
1 000	0.0	0.0	0.0	1.0	0.20	0.6
2 000	-0.1	-0.1	-0.1	2.0	0.20	0.6
4 000	-0.4	-0.4	-0.1	3.0	0.20	0.6
8 000	-0.6	-0.6	-0.2	5.0	0.20	0.7

Date of Calibration : 24-27 Feb.2025

4 / 9

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.5

Head Office
 35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
 Changwat Pathumthani 12120, Thailand
 Tel. (66) 0 2577 9036
 Fax. (66) 0 2577 9009

Office/Laboratory
 668 Mu 2 Tambon Bangpoornai, Amphoe Muang Samutprakan,
 Changwat Samutprakan 10280, Thailand
 Tel. (66) 0 2323 1672-80 ext. 115, 116
 (66) 08 3219 9440
 E-mail : mtg@tistr.or.th Website : www.tistr.or.th

Office
 196 Phahonyothin Road, Ladyao, Chatuchak,
 Bangkok 10900, Thailand
 Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
 (66) 08 1889 6827

7. Level linearity on the reference level range

Anticipated value (dB)	Measured Value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
122	122.0	0.0	1.1	0.30	0.3
121	121.0	0.0	1.1	0.30	0.3
120	120.0	0.0	1.1	0.30	0.3
119	119.0	0.0	1.1	0.30	0.3
114	114.0	0.0	1.1	0.30	0.3
109	109.0	0.0	1.1	0.30	0.3
104	104.0	0.0	1.1	0.30	0.3
99	99.0	0.0	1.1	0.30	0.3
94	94.0	0.0	1.1	0.30	0.3
89	89.0	0.0	1.1	0.30	0.3
84	84.1	0.1	1.1	0.30	0.3
79	79.1	0.1	1.1	0.30	0.3
74	74.1	0.1	1.1	0.30	0.3
69	69.1	0.1	1.1	0.30	0.3
64	64.0	0.0	1.1	0.30	0.3
59	59.0	0.0	1.1	0.30	0.3
54	54.0	0.0	1.1	0.30	0.3
49	49.0	0.0	1.1	0.30	0.3
44	44.0	0.0	1.1	0.30	0.3
39	39.0	0.0	1.1	0.30	0.3
34	34.1	0.1	1.1	0.30	0.3
33	33.1	0.1	1.1	0.30	0.3

Date of Calibration : 24-27 Feb.2025

6 / 9

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.5

Head Office
 35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
 Changwat Pathumthani 12120, Thailand
 Tel. (66) 0 2577 9036
 Fax. (66) 0 2577 9009

Office/Laboratory
 668 Mu 2 Tambon Bangpoornai, Amphoe Muang Samutprakan,
 Changwat Samutprakan 10280, Thailand
 Tel. (66) 0 2323 1672-80 ext. 115, 116
 (66) 08 3219 9440
 E-mail : mtg@tistr.or.th Website : www.tistr.or.th

Office
 196 Phahonyothin Road, Ladyao, Chatuchak,
 Bangkok 10900, Thailand
 Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
 (66) 08 1889 6827

5. Long-term stability

Time	Measured Value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Begin	94.0	0.0	0.3	0.10	0.1
End	94.0				

6. Frequency and time weightings at 1 kHz
6.1 Frequency weightings at 1 kHz

Frequency Weighting	Measured Value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
A-weight	94.0	0.0	0.2	0.20	0.2
C-weight	94.0	0.0	0.2	0.20	0.2
Flat	94.0	0.0	0.2	0.20	0.2

6.2 Time weightings at 1 kHz

Frequency Weighting	Measured Value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Fast	94.0	0.0	0.1	0.20	0.2
Slow	94.0	0.0	0.1	0.20	0.2
Leq	94.0	0.0	0.1	0.20	0.2

Date of Calibration : 24-27 Feb.2025

5 / 9

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.5

Head Office
 35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
 Changwat Pathumthani 12120, Thailand
 Tel. (66) 0 2577 9036
 Fax. (66) 0 2577 9009

Office/Laboratory
 668 Mu 2 Tambon Bangpoornai, Amphoe Muang Samutprakan,
 Changwat Samutprakan 10280, Thailand
 Tel. (66) 0 2323 1672-80 ext. 115, 116
 (66) 08 3219 9440
 E-mail : mtg@tistr.or.th Website : www.tistr.or.th

Office
 196 Phahonyothin Road, Ladyao, Chatuchak,
 Bangkok 10900, Thailand
 Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
 (66) 08 1889 6827

7. Level linearity on the reference level range

Anticipated value (dB)	Measured Value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
32	32.2	0.2	1.1	0.30	0.3
31	31.2	0.2	1.1	0.30	0.3
30	30.3	0.3	1.1	0.30	0.3

8. Level linearity including the level range control

At reference sound level on the reference level range

Range	Anticipated value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
40-130	94.0	94.0	0.0	1.1	0.30	0.3
30-120	94.0	94.0	0.0	1.1	0.30	0.3
20-110	94.0	94.0	0.0	1.1	0.30	0.3
20-100	94.0	94.0	0.0	1.1	0.30	0.3

Date of Calibration : 24-27 Feb.2025

7 / 9

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.5

Head Office
 35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
 Changwat Pathumthani 12120, Thailand
 Tel. (66) 0 2577 9036
 Fax. (66) 0 2577 9009

Office/Laboratory
 668 Mu 2 Tambon Bangpoornai, Amphoe Muang Samutprakan,
 Changwat Samutprakan 10280, Thailand
 Tel. (66) 0 2323 1672-80 ext. 115, 116
 (66) 08 3219 9440
 E-mail : mtg@tistr.or.th Website : www.tistr.or.th

Office
 196 Phahonyothin Road, Ladyao, Chatuchak,
 Bangkok 10900, Thailand
 Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
 (66) 08 1889 6827

8. Level linearity including the level range control

At reference level at 5 dB greater than the under-range on a level range

Range	Anticipated value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
40-130	45.0	45.0	0.0	1.1	0.30	0.3
30-120	35.0	35.0	0.0	1.1	0.30	0.3
20-110	25.0	25.3	0.3	1.1	0.30	0.3
20-100	25.0	25.2	0.2	1.1	0.30	0.3
20-90	25.0	25.1	0.1	1.1	0.30	0.3
20-80	25.0	24.9	-0.1	1.1	0.30	0.3

9. Tone burst response

Time Weighting	Toneburst Duration, Tb (ms)	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Fast	200	115.8	-0.2	±1.0	0.20	0.3
	2	98.9	-0.1	+1.0; -2.5	0.20	0.3
	0.25	89.0	-1.0	+1.5; -5.0	0.20	0.3
Slow	200	109.3	-0.3	±1.0	0.20	0.3
	2	89.8	-0.2	+1.0; -5.0	0.20	0.3
SEL	200	109.9	-0.1	±1.0	0.20	0.3
	2	89.9	-0.1	+1.0; -2.5	0.20	0.3
	0.25	80.9	-0.1	+1.5; -5.0	0.20	0.3

Date of Calibration : 24-27 Feb.2025

8 / 9

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FMBL.MTC.002 Rev.5

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang, Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9009

Office/Laboratory
668 Mu 2 Tambon Bangpoojai, Amphoe Muang Samutprakan, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtctr@tistr.or.th Website : www.tistr.or.th

Office
196 Phahonyothin Road, Ladysao, Chatuchak, Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827

CALIBRATION CERTIFICATE

Submitted by : Integrated Research Center Company Limited.

Address : 122 Moo 2, T.Thatoom, A.Srimahaphote, Prachinburi 25140.

Calibrated at : Electrical and Electronic Standards Laboratory, Industrial Metrology and Testing Service Centre.
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Rd., A.Muang, Samutprakan 10280.

Instrument Calibrated :

Description : Sound Level Meter
Manufacturer : ACO
Model : 6236
Serial No. : 212016
Microphone : 7052NR No.76237
Preamplifier : -

Ambient Environment

Temperature : (23 ± 3) °C
Relative Humidity : (50 ± 15) %
Ambient Pressure : (101.325±1.5) kPa

Standards used :

1. Band Pass Filter Stanford Research Systems SR 650 S/N 28712.
2. Condenser Microphone Brüel&Kjær 4180 S/N 2889871.
3. Decade Attenuator Ando AL-205 S/N 00464602.
4. Function/Arbitrary Waveform Generator Agilent 33220A S/N MY44042668.
5. Digital Function Synthesizer NF Electronic Instruments DF-193A S/N 122037.
6. Sound Calibrator Brüel&Kjær 4231 S/N 3015154.
7. Measuring Amplifier Brüel&Kjær 2636 S/N 1537484.

Date of Receipt : 14 Jan.2025

Date of Calibration : 24-27 Feb.2025

1 / 9

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FMBL.MTC.002 Rev.5

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang, Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9009

Office/Laboratory
668 Mu 2 Tambon Bangpoojai, Amphoe Muang Samutprakan, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtctr@tistr.or.th Website : www.tistr.or.th

Office
196 Phahonyothin Road, Ladysao, Chatuchak, Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827

10. Peak C sound level

Number of cycles in test signal	Anticipated value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Complete cycle	125.4	125.5	0.1	3.0	0.20	0.35
Positive half cycle	124.4	124.3	-0.1	2.0	0.20	0.35
Negative half cycle	124.4	124.3	-0.1	2.0	0.20	0.35

11. Overload indication

Measured value (dB)		Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Positive one-half cycle	Negative one-half cycle				
132.5	132.5	0.0	1.5	0.20	0.25

12. High-level stability

Time	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Begin	129.0	0.0	0.3	0.10	0.1
End	129.0				

Calibrated by :

(Signature)
.....
(Mr. Tawikiat Jamsamran)

Approved by :

(Signature)
.....
(Mr. Pravee Khasaypa)
Director

Electrical and Electronic Standards Laboratory

Industrial Metrology and Testing Service Centre

Date of Calibration : 24-27 Feb.2025

Date of Issue : 28 Feb.2025

Ref: 2011268011400185005

End of Certificate

9 / 9

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FMBL.MTC.002 Rev.5

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang, Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9009

Office/Laboratory
668 Mu 2 Tambon Bangpoojai, Amphoe Muang Samutprakan, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtctr@tistr.or.th Website : www.tistr.or.th

Office
196 Phahonyothin Road, Ladysao, Chatuchak, Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827

8. Power Amplifier Brüel&Kjær 2706 S/N 1517650.
9. Speaker Tannoy Limited, Great Britain British Patent No. 215300.
10. Digital Multimeter Agilent 34401A S/N MY44005560.
11. Programmable Attenuator Tamagawa TPA-303A S/N 2212.

Calibration Procedure :

This instrument was calibrated by using calibration procedures no CP-102-02 and CP-102-03, which were based on IEC 61672-3 Electroacoustics - Sound Level Meters - Part 3 : Periodic tests (2013). These calibration procedures were related to the electrical and acoustic signal tests. The electrical signal test was carried out with the direct measurement method. The acoustic signal test was performed in an anechoic room with the comparison measurement method.

This instrument has been calibrated against standards maintained at the Electrical and Electronic Standards Laboratory (EEL), which are traceable to the International System of Units through the National Institute of Metrology (Thailand).

The information on actual reading is attached herewith and the uncertainty limits quoted refer to the measured values only.

The reported expanded uncertainty is based upon a standard uncertainty multiplied by a coverage factor k=2, providing a level of confidence of approximately 95%.

Date of Calibration : 24-27 Feb.2025

2 / 9

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FMBL.MTC.002 Rev.5

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang, Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9009

Office/Laboratory
668 Mu 2 Tambon Bangpoojai, Amphoe Muang Samutprakan, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtctr@tistr.or.th Website : www.tistr.or.th

Office
196 Phahonyothin Road, Ladysao, Chatuchak, Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827

1. Absolute Sensitivity

Reference Acoustic Signal (dB)	Measured value (dB)	Deviation value (dB)	Acceptance limit Class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
93.99	94.0	0.0	1.0	0.48	N/A

Note: No adjustment.

2. Self-generated noise
2.1 Normal test

Measured value (dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
21.3	0.10	N/A

2.2 The microphone of the sound level meter was replaced by electrical signal input device

Frequency Weighting	Measured value (dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
A-Weight	14.4	0.10	N/A
C-Weight	19.1	0.10	N/A
Flat	23.5	0.10	N/A

Date of Calibration : 24-27 Feb.2025

3 / 9

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FMBL.MTC.002 Rev.5

Head Office
 35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang, Changwat Pathumthani 12120, Thailand
 Tel. (66) 0 2577 9036
 Fax. (66) 0 2577 9009

Office/Laboratory
 668 Mu 2 Tambon Bangpoornai, Amphoe Muang Samutprakan, Changwat Samutprakan 10280, Thailand
 Tel. (66) 0 2323 1672-80 ext. 115, 116
 (66) 08 3219 9400
 E-mail : mtc@tistr.or.th Website : www.tistr.or.th

Office
 196 Phahonyothin Road, Ladysao, Chachak, Bangkok 10900, Thailand
 Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
 (66) 08 1889 6827

5. Long-term stability

Time	Measured Value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Begin	94.0	0.0	0.3	0.10	0.1
End	94.0				

6. Frequency and time weightings at 1 kHz
6.1 Frequency weightings at 1 kHz

Frequency Weighting	Measured Value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
A-weight	94.0	0.0	0.2	0.20	0.2
C-weight	94.0	0.0	0.2	0.20	0.2
Flat	94.0	0.0	0.2	0.20	0.2

6.2 Time weightings at 1 kHz

Frequency Weighting	Measured Value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Fast	94.0	0.0	0.1	0.20	0.2
Slow	94.0	0.0	0.1	0.20	0.2
Leq	94.0	0.0	0.1	0.20	0.2

Date of Calibration : 24-27 Feb.2025

5 / 9

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FMBL.MTC.002 Rev.5

Head Office
 35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang, Changwat Pathumthani 12120, Thailand
 Tel. (66) 0 2577 9036
 Fax. (66) 0 2577 9009

Office/Laboratory
 668 Mu 2 Tambon Bangpoornai, Amphoe Muang Samutprakan, Changwat Samutprakan 10280, Thailand
 Tel. (66) 0 2323 1672-80 ext. 115, 116
 (66) 08 3219 9400
 E-mail : mtc@tistr.or.th Website : www.tistr.or.th

Office
 196 Phahonyothin Road, Ladysao, Chachak, Bangkok 10900, Thailand
 Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
 (66) 08 1889 6827

3. Acoustical signal test of frequency weightings

Frequency (Hz)	Deviation from frequency response (dB)			Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
	A-weight	C-weight	Flat			
125	0.5	0.5	0.4	1.5	0.45	0.6
1 000	-0.1	-0.1	0.0	1.0	0.45	0.6
8 000	-1.5	-1.7	-1.1	5.0	0.45	0.7

4. Electrical signal test of frequency weightings

Frequency (Hz)	Deviation from frequency response (dB)			Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
	A-weight	C-weight	Flat			
63	0.1	0.0	-0.1	2.0	0.20	0.6
125	0.0	0.0	0.0	1.5	0.20	0.6
250	0.0	0.0	0.0	1.5	0.20	0.6
500	0.0	0.0	0.0	1.5	0.20	0.6
1 000	0.0	0.0	0.0	1.0	0.20	0.6
2 000	-0.1	0.0	-0.1	2.0	0.20	0.6
4 000	-0.4	-0.3	-0.1	3.0	0.20	0.6
8 000	-0.6	-0.6	-0.2	5.0	0.20	0.7

Date of Calibration : 24-27 Feb.2025

4 / 9

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FMBL.MTC.002 Rev.5

Head Office
 35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang, Changwat Pathumthani 12120, Thailand
 Tel. (66) 0 2577 9036
 Fax. (66) 0 2577 9009

Office/Laboratory
 668 Mu 2 Tambon Bangpoornai, Amphoe Muang Samutprakan, Changwat Samutprakan 10280, Thailand
 Tel. (66) 0 2323 1672-80 ext. 115, 116
 (66) 08 3219 9400
 E-mail : mtc@tistr.or.th Website : www.tistr.or.th

Office
 196 Phahonyothin Road, Ladysao, Chachak, Bangkok 10900, Thailand
 Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
 (66) 08 1889 6827

7. Level linearity on the reference level range

Anticipated value (dB)	Measured Value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
122	122.1	0.1	1.1	0.30	0.3
121	121.1	0.1	1.1	0.30	0.3
120	120.1	0.1	1.1	0.30	0.3
119	119.1	0.1	1.1	0.30	0.3
114	114.0	0.0	1.1	0.30	0.3
109	109.0	0.0	1.1	0.30	0.3
104	104.0	0.0	1.1	0.30	0.3
99	99.0	0.0	1.1	0.30	0.3
94	94.0	0.0	1.1	0.30	0.3
89	89.0	0.0	1.1	0.30	0.3
84	83.9	-0.1	1.1	0.30	0.3
79	78.9	-0.1	1.1	0.30	0.3
74	74.1	0.1	1.1	0.30	0.3
69	69.2	0.2	1.1	0.30	0.3
64	64.0	0.0	1.1	0.30	0.3
59	59.0	0.0	1.1	0.30	0.3
54	54.0	0.0	1.1	0.30	0.3
49	49.1	0.1	1.1	0.30	0.3
44	44.1	0.1	1.1	0.30	0.3
39	39.0	0.0	1.1	0.30	0.3
34	34.2	0.2	1.1	0.30	0.3
33	33.2	0.2	1.1	0.30	0.3

Date of Calibration : 24-27 Feb.2025

6 / 9

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FMBL.MTC.002 Rev.5

Head Office
 35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang, Changwat Pathumthani 12120, Thailand
 Tel. (66) 0 2577 9036
 Fax. (66) 0 2577 9009

Office/Laboratory
 668 Mu 2 Tambon Bangpoornai, Amphoe Muang Samutprakan, Changwat Samutprakan 10280, Thailand
 Tel. (66) 0 2323 1672-80 ext. 115, 116
 (66) 08 3219 9400
 E-mail : mtc@tistr.or.th Website : www.tistr.or.th

Office
 196 Phahonyothin Road, Ladysao, Chachak, Bangkok 10900, Thailand
 Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
 (66) 08 1889 6827

7. Level linearity on the reference level range

Anticipated value (dB)	Measured Value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
32	32.2	0.2	1.1	0.30	0.3
31	31.2	0.2	1.1	0.30	0.3
30	30.3	0.3	1.1	0.30	0.3

8. Level linearity including the level range control

At reference sound level on the reference level range

Range	Anticipated value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
40-130	94.0	94.0	0.0	1.1	0.30	0.3
30-120	94.0	94.0	0.0	1.1	0.30	0.3
20-110	94.0	94.0	0.0	1.1	0.30	0.3
20-100	94.0	94.0	0.0	1.1	0.30	0.3

Date of Calibration : 24-27 Feb.2025

7 / 9

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FMBL.MTC.002 Rev.5

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang, Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9009

Office/Laboratory
668 Mu 2 Tambon Bangpoornai, Amphoe Muang Samutprakarn, Changwat Samutprakarn 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtic@tistr.or.th Website : www.tistr.or.th

Office
196 Phahonyothin Road, Ladysao, Chatuchak, Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 52217
(66) 08 1889 6827

10. Peak C sound level

Number of cycles in test signal	Anticipated value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Complete cycle	125.4	125.3	-0.1	3.0	0.20	0.35
Positive half cycle	124.4	124.3	-0.1	2.0	0.20	0.35
Negative half cycle	124.4	124.2	-0.2	2.0	0.20	0.35

11. Overload indication

Measured value (dB)		Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Positive one-half cycle	Negative one-half cycle				
132.5	132.5	0.0	1.5	0.20	0.25

12. High-level stability

Time	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Begin	129.0	0.0	0.3	0.10	0.1
End	129.0				

Calibrated by : *Suk A.*
(Mr. Tawikiat Iamsamran)

Approved by : *Prawate Klaiyapa*
(Mr. Prawate Klaiyapa)
Director

Electrical and Electronic Standards Laboratory
Industrial Metrology and Testing Service Centre

Date of Calibration : 24-27 Feb.2025

Date of Issue : 28 Feb.2025

Ref : 2011268011400185006

End of Certificate

9 / 9

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FMBL.MTC.002 Rev.5

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang, Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9009

Office/Laboratory
668 Mu 2 Tambon Bangpoornai, Amphoe Muang Samutprakarn, Changwat Samutprakarn 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtic@tistr.or.th Website : www.tistr.or.th

Office
196 Phahonyothin Road, Ladysao, Chatuchak, Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 52217
(66) 08 1889 6827

8. Level linearity including the level range control

At reference level at 5 dB greater than the under-range on a level range

Range	Anticipated value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
40-130	45.0	45.0	0.0	1.1	0.30	0.3
30-120	35.0	35.0	0.0	1.1	0.30	0.3
20-110	25.0	25.5	0.5	1.1	0.30	0.3
20-100	25.0	25.4	0.4	1.1	0.30	0.3
20-90	25.0	25.3	0.3	1.1	0.30	0.3
20-80	25.0	25.2	0.2	1.1	0.30	0.3

9. Tone burst response

Time Weighting	Toneburst Duration, Tb (ms)	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Fast	200	115.9	-0.1	±1.0; -2.5	0.20	0.3
	2	98.1	-0.9	+1.0; -2.5	0.20	0.3
	0.25	89.2	-0.8	+1.5; -5.0	0.20	0.3
Slow	200	109.5	-0.1	±1.0	0.20	0.3
	2	89.8	-0.2	+1.0; -5.0	0.20	0.3
SEL	200	109.9	-0.1	±1.0	0.20	0.3
	2	90.0	0.0	+1.0; -2.5	0.20	0.3
	0.25	80.9	-0.1	+1.5; -5.0	0.20	0.3

Date of Calibration : 24-27 Feb.2025

8 / 9

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FMBL.MTC.002 Rev.5

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang, Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9009

Office/Laboratory
668 Mu 2 Tambon Bangpoornai, Amphoe Muang Samutprakarn, Changwat Samutprakarn 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtic@tistr.or.th Website : www.tistr.or.th

Office
196 Phahonyothin Road, Ladysao, Chatuchak, Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 52217
(66) 08 1889 6827



Airgas Specialty Gases
Airgas USA, LLC
600 Union Landing Road
Cinnaminson, NJ 08077-0000
Airgas.com

CERTIFICATE OF ANALYSIS
Grade of Product: EPA Protocol

Part Number: E03N899E80A0020 Reference Number: 82-401285019-1
Cylinder Number: LL193324 Cylinder Volume: 83.4 CF
Laboratory: 124 - Riverton (SAP) - NJ Cylinder Pressure: 2215 PSIG
PGVP Number: B52018 Valve Outlet: 660
Gas Code: NO,NOX,SO2,BALN Certification Date: Sep 05, 2018

Expiration Date: Sep 05, 2026

Certification performed in accordance with EPA Traceability Protocol for Assay and Certification of Gaseous Calibration Standards (May 2012) document EPA 600/R-12/021. Using the assay procedures listed. Analytical Methodology does not require correction for analytical interference. This cylinder has a total analytical uncertainty as stated below with a confidence level of 95%. There are no significant impurities which affect the use of this calibration mixture. All concentrations are on a volume/volume basis unless otherwise noted.
Do Not Use This Cylinder below 100 psig, i.e. 0.7 megapascals.

ANALYTICAL RESULTS						
Component	Requested Concentration	Actual Concentration	Protocol Method	Total Relative Uncertainty	Assay Dates	
NOX	50.00 PPM	50.71 PPM	G1	±1.4% NIST Traceable	08/27/2018, 09/05/2018	
NITRIC OXIDE	50.00 PPM	50.67 PPM	G1	±1.4% NIST Traceable	08/27/2018, 09/05/2018	
SULFUR DIOXIDE	50.00 PPM	50.54 PPM	G1	±1.0% NIST Traceable	08/27/2018, 09/05/2018	
NITROGEN	Balance					

CALIBRATION STANDARDS						
Type	Lot ID	Cylinder No	Concentration	Uncertainty	Expiration Date	
NTRM	16060525	CC442585	50.42 PPM NITRIC OXIDE/NITROGEN	±1.0%	Jun 27, 2020	
PRM	12368	5604119	29.86 PPM NITROGEN DIOXIDE/AIR	±1.5%	Jun 02, 2017	
GMIS	7042010104	CC503941	5.101 PPM NITROGEN DIOXIDE/NITROGEN	±1.0%	Jun 01, 2020	
NTRM	14010327	KAL004378	49.08 PPM SULFUR DIOXIDE/NITROGEN	±1.0%	Apr 17, 2024	

The SRM, PRM or RGM noted above is only in reference to the GMS used in the assay and not part of the analysis.

ANALYTICAL EQUIPMENT		
Instrument/Make/Model	Analytical Principle	Last Multipoint Calibration
Nicomet 6700 APW1100391 NO	FTIR	Aug 09, 2018
Nicomet 6700 APW1100391 NO2	FTIR	Aug 31, 2018
Nicomet 6700 APW1100391 SO2	FTIR	Aug 30, 2018

Triad Data Available Upon Request
NOTES: PO# 5218003935

Net weight: 2736 grams
Gross weight: 17393 grams

This calibration std. has been certified in accordance with the May 2012 EPA Traceability Protocol Document EPA-600/R-12/031. All testing processes and measurements conform to the requirements of ISO/IEC 17025 and to Airgas ISO 9001:2008 and relate only to items identified on this certificate. Values are certified to be NIST Traceable with total uncertainty as detailed under Analytical Uncertainty. This document shall not be reproduced in full without written approval of the issuer.



TESTING CERT No. 3082.05

Approved for Release

CERTIFICATE OF ANALYSIS
Grade of Product: EPA Protocol

Part Number: E03N899E80A0020 Reference Number: 82-401285019-1
 Cylinder Number: LL193324 Cylinder Volume: 83.4 CF
 Laboratory: 124 - Rverton (SAP) - NJ Cylinder Pressure: 2215 PSIG
 PGVP Number: B52018 Valve Outlet: 660
 Gas Code: NO,NOX,SO2,BALN Certification Date: Sep 05, 2018
 Expiration Date: **Sep 05, 2026**

Certification performed in accordance with "EPA Traceability Protocol for Assay and Certification of Gaseous Calibration Standards (May 2012)" document EPA 600/R-12/531, using the assay procedures listed. Analytical Methodology does not require correction for analytical interference. This cylinder has a total analytical uncertainty as stated below with a confidence level of 95%. There are no significant impurities which affect the use of this calibration mixture. All concentrations are on a volume/volume basis unless otherwise noted.
 Do Not Use This Cylinder below 100 psig, i.e. 0.7 megapascals.

ANALYTICAL RESULTS

Component	Requested Concentration	Actual Concentration	Protocol Method	Total Relative Uncertainty	Assay Dates
NOX	50.00 PPM	50.71 PPM	G1	+/- 1.4% NIST Traceable	08/27/2018, 09/05/2018
NITRIC OXIDE	50.00 PPM	50.67 PPM	G1	+/- 1.4% NIST Traceable	08/27/2018, 09/05/2018
SULFUR DIOXIDE	50.00 PPM	50.54 PPM	G1	+/- 1.0% NIST Traceable	08/27/2018, 09/05/2018
NITROGEN	Balance				

CALIBRATION STANDARDS

Type	Lot ID	Cylinder No	Concentration	Uncertainty	Expiration Date
NTRM	16050525	CC442585	50.42 PPM NITRIC OXIDE/NITROGEN	+/- 0.8%	Jun 27, 2020
PRM	12368	5604119	29.86 PPM NITROGEN DIOXIDE/AIR	+/- 1.5%	Jun 02, 2017
GMS	7042010104	CC503941	5.101 PPM NITROGEN DIOXIDE/NITROGEN	+/- 2.0%	Jun 01, 2020
NTRM	14010327	KAL004378	49.08 PPM SULFUR DIOXIDE/NITROGEN	+/- 1.0%	Apr 17, 2024

The SRM, PRM or RGM noted above is only in reference to the GMS used in the assay and not part of the analysis.

ANALYTICAL EQUIPMENT

Instrument/Make/Model	Analytical Principle	Last Multipoint Calibration
Nicodet 6700 APW1100391 NO	FTIR	Aug 09, 2018
Nicodet 6700 APW1100391 NO2	FTIR	Aug 31, 2018
Nicodet 6700 APW1100391 SO2	FTIR	Aug 30, 2018

Triad Data Available Upon Request

NOTES: PO# 5218003935

Net weight: 2736 grams
Gross weight: 17393 grams

This calibration std. has been certified in accordance with the May 2012 EPA Traceability Protocol Document EPA-600/R-12/531. All testing processes and measurements conform to the requirements of ISO/IEC 17025 and to Airgas ISO 9001:2008 and relate only to items identified on this certificate. We are certified to be NIST Traceable with total uncertainty as detailed under Analytical Uncertainty. This document shall not be reproduced in full without written approval of the issuer.



TESTING CERT No. 3082.05

[Signature]
Approved for Release

ภาคผนวก ฉ
สำเนาหนังสืออนุญาตขึ้นทะเบียน
ห้องปฏิบัติการวิเคราะห์เอกชน

บริษัท ยูไนเต็ด แอนนาลิสต์ แอนด์ เอ็นจิเนียริง
คอนซัลแตนท์ จำกัด



ที่ อก ๐๓๑๐(๑)/ ๑๐๘๕

กรมโรงงานอุตสาหกรรม
ถนนพระรามที่ ๖ แขวงทุ่งพญาไท
เขตราชเทวี กรุงเทพฯ ๑๐๕๐๐

๐๗ กุมภาพันธ์ ๒๕๖๕

เรื่อง ต่ออายุหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน
เรียน กรรมการผู้จัดการ บริษัท ยูโนเด็ค แอนนาลิสต์ แอนด์ เอ็นจิเนียริง คอนซัลแตนท์ จำกัด
อ้างถึง คำขอขึ้นทะเบียน/ต่ออายุ/เปลี่ยนแปลงบุคลากร และขอใบสารมลพิษของห้องปฏิบัติการวิเคราะห์เอกชน
ลงวันที่ ๓ ธันวาคม ๒๕๖๔

สิ่งที่ส่งมาด้วย ๓. รายชื่อผู้ควบคุมห้องปฏิบัติการวิเคราะห์เอกชน จำนวน ๔๐ ราย
๒. รายชื่อเจ้าหน้าที่ห้องปฏิบัติการวิเคราะห์เอกชน จำนวน ๑๔๓ ราย
๓. ขอบข่ายสารมลพิษที่ได้รับขึ้นทะเบียนจากกรมโรงงานอุตสาหกรรม
ตามคำขอที่อ้างถึง บริษัท ยูโนเด็ค แอนนาลิสต์ แอนด์ เอ็นจิเนียริง คอนซัลแตนท์ จำกัด ขอต่ออายุ
หนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน เลขทะเบียน ๖-๑๔๕ สถานที่ยื่นเลขที่ ๓ ซอยสุขุมสุข ๕๓
ถนนสุขุมวิท แขวงบางจาก เขตพระโขนง กรุงเทพมหานคร ต่อกรมโรงงานอุตสาหกรรม นั้น

กรมโรงงานอุตสาหกรรมพิจารณาแล้ว ให้บริษัท ยูโนเด็ค แอนนาลิสต์ แอนด์ เอ็นจิเนียริง
คอนซัลแตนท์ จำกัด ต่ออายุหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน โดยมีองค์ประกอบดังนี้

- ก. ผู้ควบคุมห้องปฏิบัติการวิเคราะห์เอกชน จำนวน ๔๐ ราย ตามสิ่งที่ส่งมาด้วย ๓
- ข. เจ้าหน้าที่ห้องปฏิบัติการวิเคราะห์เอกชน จำนวน ๑๔๓ ราย ตามสิ่งที่ส่งมาด้วย ๒
- ค. ขอบข่ายสารมลพิษที่ได้รับขึ้นทะเบียนให้วิเคราะห์ในน้ำ/น้ำเสีย น้ำใต้ดิน อากาศเสีย
สิ่งปฏิกูลหรือวัสดุที่ไม่ใช้แล้ว และดิน ตามสิ่งที่ส่งมาด้วย ๓

หนังสือฉบับนี้จะหมดอายุในวันที่ ๒ กุมภาพันธ์ ๒๕๖๖ หากประสงค์จะต่ออายุหนังสือ
รับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน ให้ยื่นคำขอต่ออายุพร้อมเอกสารประกอบคำขอต่อกรมโรงงาน
อุตสาหกรรมภายใน ๖๐ วัน ก่อนวันสิ้นสุดของหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน

จึงเรียนมาเพื่อทราบ

ขอแสดงความนับถือ

(นายธีรภัทร์ อิศรางกูร ณ อยุธยา)
รองอธิบดี ปฏิบัติราชการแทน
อธิบดีกรมโรงงานอุตสาหกรรม

กองวิจัยและเตือนภัยมลพิษโรงงาน
กลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษและทะเบียนห้องปฏิบัติการ
โทร. ๐ ๒๕๓๐ ๖๓๑๒ ต่อ ๒๑๐๓-๕
โทรสาร ๐ ๒๕๓๐ ๖๓๑๖ ต่อ ๒๑๕๕
ไปรษณีย์อิเล็กทรอนิกส์ sarabang@dlw.mail.go.th



"อุตสาหกรรมก้าวไกล ประเทศไทยก้าวหน้า ร่วมกันพัฒนา อุตสาหกรรมสีเขียว"



เอกสารแนบท้ายหนังสือต่ออายุรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน
บริษัท ยูโนเด็ค แอนนาลิสต์ แอนด์ เอ็นจิเนียริง คอนซัลแตนท์ จำกัด เลขทะเบียน ๖-๑๔๕
ที่ อก ๐๓๑๐(๑)/ ๑๐๘๕ ลงวันที่ ๐๗ กุมภาพันธ์ ๒๕๖๕

ก. ผู้ควบคุมห้องปฏิบัติการวิเคราะห์เอกชน จำนวน ๔๐ ราย

- ๑) นางสาวกฤษวรรณ กิทธิกรกุล ทะเบียนเลขที่ ๖-๑๔๕-๙-๐๐๐๑
- ๒) นายณรงค์ นิมาพร ทะเบียนเลขที่ ๖-๑๔๕-๙-๐๐๐๒
- ๓) นางสาวนันทิศา บุญไชย ทะเบียนเลขที่ ๖-๑๔๕-๙-๐๐๐๓
- ๔) นางปิยะพัชร์ สุทธิธรรมสาร ทะเบียนเลขที่ ๖-๑๔๕-๙-๐๐๐๔
- ๕) นางสาวเบญจวรรณ วีริโยทัย ทะเบียนเลขที่ ๖-๑๔๕-๙-๐๐๐๖
- ๖) นายพนรัตน์ วงศ์บุรุษชัย ทะเบียนเลขที่ ๖-๑๔๕-๙-๐๐๐๗
- ๗) นางสาวฉวีวรรณ บุญลา ทะเบียนเลขที่ ๖-๑๔๕-๙-๐๐๐๘
- ๘) นายสุวิทย์ จอดนอก ทะเบียนเลขที่ ๖-๑๔๕-๙-๐๐๐๙
- ๙) นางสาวโศภิตา สมบูรณ์ ทะเบียนเลขที่ ๖-๑๔๕-๙-๐๐๑๐
- ๑๐) นางสาวบุษกร เลิศกาญจนาภักดิ์ ทะเบียนเลขที่ ๖-๑๔๕-๙-๐๐๑๑
- ๑๑) นางสาววิไลลักษณ์ ศรีสุข ทะเบียนเลขที่ ๖-๑๔๕-๙-๐๐๑๒
- ๑๒) นายศิลา บรรจงรังรักษ์ ทะเบียนเลขที่ ๖-๑๔๕-๙-๐๐๑๔
- ๑๓) นายปฏิกรณ์ คณะนา ทะเบียนเลขที่ ๖-๑๔๕-๙-๐๐๑๕
- ๑๔) นายธีรวัฒน์ ชะมิง ทะเบียนเลขที่ ๖-๑๔๕-๙-๐๐๑๖
- ๑๕) นางสาวศิริพร ศรีประดิษฐ์ ทะเบียนเลขที่ ๖-๑๔๕-๙-๐๐๑๗
- ๑๖) นางสาวสาวิตรี วีระ ทะเบียนเลขที่ ๖-๑๔๕-๙-๐๐๑๘
- ๑๗) นางสาวนพพรณ สุรารักษ์ ทะเบียนเลขที่ ๖-๑๔๕-๙-๐๐๑๙
- ๑๘) นายรุ่งรงค์ พาณิชย์เลิศอำไพ ทะเบียนเลขที่ ๖-๑๔๕-๙-๐๐๒๐
- ๑๙) นายณัฐวัฒน์ แสงสวัสดิ์ ทะเบียนเลขที่ ๖-๑๔๕-๙-๐๐๒๓
- ๒๐) นายเอกรัตน์ ปอดะคามินทร์ ทะเบียนเลขที่ ๖-๑๔๕-๙-๐๐๒๖
- ๒๑) นางสาวนิศากรัน ศรีสกุลสิทธิ์โชค ทะเบียนเลขที่ ๖-๑๔๕-๙-๐๐๒๓
- ๒๒) นางสาวเจษฎินทร์ ทาละอาด ทะเบียนเลขที่ ๖-๑๔๕-๙-๐๐๒๔
- ๒๓) นางสาวสุวรรณ คงทอง ทะเบียนเลขที่ ๖-๑๔๕-๙-๐๐๒๕
- ๒๔) นางสาววรรณ พิศลสงจิน ทะเบียนเลขที่ ๖-๑๔๕-๙-๐๐๒๖
- ๒๕) นายวิรุฬห์ โมกแก้ว ทะเบียนเลขที่ ๖-๑๔๕-๙-๐๐๒๗
- ๒๖) นายวีรพงษ์ เทพนครี ทะเบียนเลขที่ ๖-๑๔๕-๙-๐๐๒๘
- ๒๗) นายอนุศาสน์ สายดี ทะเบียนเลขที่ ๖-๑๔๕-๙-๐๐๒๙
- ๒๘) นายกรวิทย์ เขียวศรีสกุล ทะเบียนเลขที่ ๖-๑๔๕-๙-๐๐๓๐
- ๒๙) นายสุธีระ อรุณจันทร์ ทะเบียนเลขที่ ๖-๑๔๕-๙-๐๐๓๓
- ๓๐) นางสาวศศิณี อ่อนคำ ทะเบียนเลขที่ ๖-๑๔๕-๙-๐๐๓๕
- ๓๑) นางพริ้มพรรณ กอนสิน ทะเบียนเลขที่ ๖-๑๔๕-๙-๐๐๓๕
- ๓๒) นายศุภณัฐ ฐิตนภานุจัน ทะเบียนเลขที่ ๖-๑๔๕-๙-๐๐๓๖
- ๓๓) นางสาวศศิภากร เหมือนไร่ ทะเบียนเลขที่ ๖-๑๔๕-๙-๐๐๓๗
- ๓๔) นางศิวิลา ชำนิล ทะเบียนเลขที่ ๖-๑๔๕-๙-๐๐๓๘
- ๓๕) นางสาวพรรณีภา ริเชจินดาชล ทะเบียนเลขที่ ๖-๑๔๕-๙-๐๐๓๙

อนุมัติ

๓๖) นายนาเคนทร์...

- ๓๖) นายนาเคนทร์ พันธุ์ชาติกุล ทะเบียนเลขที่ ๖-๑๔๕-๙-๐๐๔๐
- ๓๗) นายกานต์พงษ์ บุญพวง ทะเบียนเลขที่ ๖-๑๔๕-๙-๐๐๔๑
- ๓๘) นางสุธรรมา แก้วชื่อนอก ทะเบียนเลขที่ ๖-๑๔๕-๙-๐๐๔๒
- ๓๙) นางสาวสรวิมล โยเซษย์พิพัฒกุล ทะเบียนเลขที่ ๖-๑๔๕-๙-๐๐๔๓
- ๔๐) นางมานิตา เข้มโย ทะเบียนเลขที่ ๖-๑๔๕-๙-๐๐๔๔

อนุมัติ

เอกสารแนบท้ายหนังสือต่ออายุรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน
บริษัท ยูโนเด็ค แอนนาลิสต์ แอนด์ เอ็นจิเนียริง คอนซัลแตนท์ จำกัด เลขทะเบียน ๖-๑๔๕
ที่ อก ๐๓๑๐(๑)/ ๑๐๘๕ ลงวันที่ ๐๗ กุมภาพันธ์ ๒๕๖๕

ข. เจ้าหน้าที่ห้องปฏิบัติการวิเคราะห์เอกชน จำนวน ๑๔๓ ราย

- ๑) นายสุธนต์ พันสิงห์ ทะเบียนเลขที่ ๖-๑๔๕-๙-๐๐๐๑
- ๒) นายพีรณัฐ เจริญผล ทะเบียนเลขที่ ๖-๑๔๕-๙-๐๐๐๓
- ๓) นางสาววิไลลักษณ์ เกโลสง ทะเบียนเลขที่ ๖-๑๔๕-๙-๐๐๐๔
- ๔) นายสมชาติ อุทุมรัตน์ ทะเบียนเลขที่ ๖-๑๔๕-๙-๐๐๐๕
- ๕) นางสาวปรมภรณ์ ทองแก้ว ทะเบียนเลขที่ ๖-๑๔๕-๙-๐๐๐๖
- ๖) นางสาวกัญญา สมพงษ์ ทะเบียนเลขที่ ๖-๑๔๕-๙-๐๐๐๗
- ๗) นางสาววรรณิ์ สายบุญเรือน ทะเบียนเลขที่ ๖-๑๔๕-๙-๐๐๑๐
- ๘) นายกฤษณพงษ์ นามทิพย์ ทะเบียนเลขที่ ๖-๑๔๕-๙-๐๐๑๑
- ๙) นางสาวอาภากรณ์ อ่อนคง ทะเบียนเลขที่ ๖-๑๔๕-๙-๐๐๑๒
- ๑๐) นายกิตติศักดิ์ ทรงจำรัส ทะเบียนเลขที่ ๖-๑๔๕-๙-๐๐๑๓
- ๑๑) นางสาวอักษรินทร์ บุญคง ทะเบียนเลขที่ ๖-๑๔๕-๙-๐๐๑๔
- ๑๒) นางสาวพรทิพย์ แก้วทอง ทะเบียนเลขที่ ๖-๑๔๕-๙-๐๐๑๕
- ๑๓) นายอภิวิชญ์ ท่วงที ทะเบียนเลขที่ ๖-๑๔๕-๙-๐๐๑๗
- ๑๔) นายมานิตย์ ปานโชติ ทะเบียนเลขที่ ๖-๑๔๕-๙-๐๐๑๘
- ๑๕) นายศพร ธนะพิรุณห์ ทะเบียนเลขที่ ๖-๑๔๕-๙-๐๐๑๙
- ๑๖) นางสาวกัญญาณี โยธา ทะเบียนเลขที่ ๖-๑๔๕-๙-๐๐๒๐
- ๑๗) นางสาวเกตุ สุทธิ ทะเบียนเลขที่ ๖-๑๔๕-๙-๐๐๒๓
- ๑๘) นางสาวชนอนัญ อภิพัทธ์ปภา ทะเบียนเลขที่ ๖-๑๔๕-๙-๐๐๒๖
- ๑๙) นายศิริพร จงพวงเกียรติ ทะเบียนเลขที่ ๖-๑๔๕-๙-๐๐๒๓
- ๒๐) นางสาวสุภาวดี อินยาศรี ทะเบียนเลขที่ ๖-๑๔๕-๙-๐๐๒๔
- ๒๑) นายพงศ์เทพ เหล่าจร ทะเบียนเลขที่ ๖-๑๔๕-๙-๐๐๒๕
- ๒๒) นายขวัญชัย พันทุภักดิ์ ทะเบียนเลขที่ ๖-๑๔๕-๙-๐๐๒๖
- ๒๓) นางสาวพัชริภา คดีพิศาล ทะเบียนเลขที่ ๖-๑๔๕-๙-๐๐๒๗
- ๒๔) นางสาวนงวิภา เสือคำจันทร์ ทะเบียนเลขที่ ๖-๑๔๕-๙-๐๐๒๘
- ๒๕) นายพีระพัฒน์ บัญญัติศิลป์ ทะเบียนเลขที่ ๖-๑๔๕-๙-๐๐๓๒
- ๒๖) นายชัชวาลย์ เลื่อนส่อง ทะเบียนเลขที่ ๖-๑๔๕-๙-๐๐๓๓
- ๒๗) นายณภินันท์ ฐุธรรมรัตน์ ทะเบียนเลขที่ ๖-๑๔๕-๙-๐๐๓๖
- ๒๘) นายกันนิกร รโยธ ทะเบียนเลขที่ ๖-๑๔๕-๙-๐๐๓๗
- ๒๙) นายปริญญา กมลเกษียา ทะเบียนเลขที่ ๖-๑๔๕-๙-๐๐๓๘
- ๓๐) นายธีรวัฒน์ มาระโพธิ์ศรี ทะเบียนเลขที่ ๖-๑๔๕-๙-๐๐๔๐
- ๓๑) นายบุญฤกษ์ ก้อนสิน ทะเบียนเลขที่ ๖-๑๔๕-๙-๐๐๔๑
- ๓๒) นายพรชบุศย์ ไกรสกุล ทะเบียนเลขที่ ๖-๑๔๕-๙-๐๐๔๓
- ๓๓) นายอชิตะ แสงจันทร์ ทะเบียนเลขที่ ๖-๑๔๕-๙-๐๐๔๔
- ๓๔) ว่าที่ร้อยตรีณัฐพงศ์ เมื่องชัย ทะเบียนเลขที่ ๖-๑๔๕-๙-๐๐๔๕
- ๓๕) นายอนันต์ เลิศประเสริฐ ทะเบียนเลขที่ ๖-๑๔๕-๙-๐๐๔๖

อนุมัติ

๓๖) นางสาวนิภาพร...

- ๓๖) นางสาวนิภาพร จันทเขตต์
- ๓๗) นายรณภพ ภูตระกูลพัฒนา
- ๓๘) นายสมพงษ์ สกุลไทย
- ๓๙) นายสุวิวัฒน์ นิธิจิตชูวงศ์
- ๔๐) นายอิชฎิภาวธ ยนศิริ
- ๔๑) นายเอกภูมิ เสนอใจ
- ๔๒) นายสุชสิทธิ์ บุญเลี้ยง
- ๔๓) นายอนันต์ หวานเสนาะ
- ๔๔) นายอภิสิทธิ์ ศรีวงแก้ว
- ๔๕) ว่าที่ร้อยตรีสุชัย แก้ววราภุมุข
- ๔๖) นางสาวนารินทร์ สานนท์
- ๔๗) นายศุภกร รัตนวงศ์
- ๔๘) นางสาวจินตสุภา เปลี่ยนศรี
- ๔๙) นางสาวเนตรนภา กมลบุรินทร์
- ๕๐) นางสาวอรวิภา พรหมรัมย์
- ๕๑) นายจิรวัฒน์ สุขเกษม
- ๕๒) นายกิตติพงษ์ สอนชัยภูมิ
- ๕๓) นายจุมพล สวนเพชร
- ๕๔) นางสาวพัชรภรณ์ แสงฟ้า
- ๕๕) นายวิวัฒน์ เหล่ามา
- ๕๖) นายอิทธิพงษ์ ศรีวิเศษ
- ๕๗) นางสาวกรรณิการ์ ลำสีทา
- ๕๘) นางสาวณัฐชา พรหมศิริ
- ๕๙) นายณสิทธิ์ ศรีพิมพ์
- ๖๐) นางสาวลลิตาภา จันทรสฤษ
- ๖๑) นายศักดิ์ศิรินทร์ นุ่มนัม
- ๖๒) นายวรพงษ์ นพจินทร์
- ๖๓) นางสาวชนภา มาคมมาตร
- ๖๔) นายณัฐชัช พรหมอารักษ์
- ๖๕) นายชินนทร์ พานแก้ว
- ๖๖) นายปรัชชาติ ไสภา
- ๖๗) นายวัชรินทร์ แสงงาม
- ๖๘) นายอาทิตย์ อุดมผล
- ๖๙) นายอิทธิเดช ใจบุญ
- ๗๐) นายณณิติน พงษ์ศรีราษฎร์
- ๗๑) นายเสฏฐวุฒิ เอมกลิ่นบัว
- ๗๒) นางสาวนาคาชา หวานโนเมือง
- ๗๓) นางสาวพิมพ์วรรณ ลิ้มมา

- ทะเบียนเลขที่ ๖-๒๕๕-๖-๐๐๔๗
- ทะเบียนเลขที่ ๖-๒๕๕-๖-๐๐๔๘
- ทะเบียนเลขที่ ๖-๒๕๕-๖-๐๐๕๑
- ทะเบียนเลขที่ ๖-๒๕๕-๖-๐๐๕๒
- ทะเบียนเลขที่ ๖-๒๕๕-๖-๐๐๕๓
- ทะเบียนเลขที่ ๖-๒๕๕-๖-๐๐๕๔
- ทะเบียนเลขที่ ๖-๒๕๕-๖-๐๐๕๕
- ทะเบียนเลขที่ ๖-๒๕๕-๖-๐๐๕๖
- ทะเบียนเลขที่ ๖-๒๕๕-๖-๐๐๕๗
- ทะเบียนเลขที่ ๖-๒๕๕-๖-๐๐๕๘
- ทะเบียนเลขที่ ๖-๒๕๕-๖-๐๐๖๐
- ทะเบียนเลขที่ ๖-๒๕๕-๖-๐๐๖๑
- ทะเบียนเลขที่ ๖-๒๕๕-๖-๐๐๖๒
- ทะเบียนเลขที่ ๖-๒๕๕-๖-๐๐๖๓
- ทะเบียนเลขที่ ๖-๒๕๕-๖-๐๐๖๔
- ทะเบียนเลขที่ ๖-๒๕๕-๖-๐๐๖๕
- ทะเบียนเลขที่ ๖-๒๕๕-๖-๐๐๖๖
- ทะเบียนเลขที่ ๖-๒๕๕-๖-๐๐๖๗
- ทะเบียนเลขที่ ๖-๒๕๕-๖-๐๐๖๘
- ทะเบียนเลขที่ ๖-๒๕๕-๖-๐๐๖๙
- ทะเบียนเลขที่ ๖-๒๕๕-๖-๐๐๗๐
- ทะเบียนเลขที่ ๖-๒๕๕-๖-๐๐๗๑
- ทะเบียนเลขที่ ๖-๒๕๕-๖-๐๐๗๒
- ทะเบียนเลขที่ ๖-๒๕๕-๖-๐๐๗๓
- ทะเบียนเลขที่ ๖-๒๕๕-๖-๐๐๗๔
- ทะเบียนเลขที่ ๖-๒๕๕-๖-๐๐๗๕
- ทะเบียนเลขที่ ๖-๒๕๕-๖-๐๐๗๖
- ทะเบียนเลขที่ ๖-๒๕๕-๖-๐๐๗๗
- ทะเบียนเลขที่ ๖-๒๕๕-๖-๐๐๗๘
- ทะเบียนเลขที่ ๖-๒๕๕-๖-๐๐๗๙
- ทะเบียนเลขที่ ๖-๒๕๕-๖-๐๐๘๐

๓๙๕

๓๙) นายบัณฑิต...

- ๓๙๖) นายบัณฑิต วงศ์คำ
- ๓๙๗) นายประพันธ์ฤทธิ์ เมื่อนาง
- ๓๙๘) นางสาวณัฐชา ลำซัด
- ๓๙๙) นางสาวนภาพร ชื่นนุกัม
- ๔๐๐) นางสาวบุญญา นอมฤต
- ๔๐๑) นายอมรพล อรรถลักษณ์
- ๔๐๒) นางสาวศรินทร์ ทองขาว
- ๔๐๓) นางสาวณิชากร คุณชาติภิรต
- ๔๐๔) นางสาววิมลวรรณ คำตัน
- ๔๐๕) นายคุณานนท์ ฤทธาคนานนท์
- ๔๐๖) นายชาญณรงค์ อ้ายลอย
- ๔๐๗) นางสาวยุติ โปชนิเงิน
- ๔๐๘) นายเจษฎา ช่างทวี
- ๔๐๙) นายยศ เหมชอุณ
- ๔๑๐) นายสุเชษฐ์ หล้าโท
- ๔๑๑) นายชัย บัวค
- ๔๑๒) นางสาวอรุणा ประสานศรี
- ๔๑๓) นายพศล เนียมเนียม
- ๔๑๔) นายศุภกร สวนศรี
- ๔๑๕) นายคณพล ศิลานนท์
- ๔๑๖) นายโชคชัย ทุมไธ
- ๔๑๗) นายธีรวัฒน์ อรรณสุวรรณ
- ๔๑๘) นายนิธพงษ์ ชะชุมทศ
- ๔๑๙) นางสาวณัฐกานา พลนิกรกิจ
- ๔๒๐) นางสาวนภาพร ทองบุญ
- ๔๒๑) นางสาวพริษา ขจรเนติสุข
- ๔๒๒) นางสาวเพ็ญพิชชา รอดทอง
- ๔๒๓) นางสาวณัฐชา แสงสว่าง
- ๔๒๔) นายกรติ สีอาจ
- ๔๒๕) นายศุภพร ศรีศรี
- ๔๒๖) นางสาวสุลลิสรา เลี่ยนเงิน
- ๔๒๗) นางสาวพรหมทิพา อะโนนาม
- ๔๒๘) นายอนันต์ มุดอ
- ๔๒๙) นางสาวพรพิบล ประชาพันธุ์
- ๔๓๐) นายวีรภัทร บุญฤทธิ
- ๔๓๑) นางสาวณัฐชา แก้วภาพ
- ๔๓๒) นายสิทธิพล พร้อมเชื้อไขบุญ
- ๔๓๓) นางสาวนันทิชา กลิ่นหนู

- ทะเบียนเลขที่ ๖-๒๕๕-๖-๐๐๑๑
- ทะเบียนเลขที่ ๖-๒๕๕-๖-๐๐๑๒
- ทะเบียนเลขที่ ๖-๒๕๕-๖-๐๐๑๓
- ทะเบียนเลขที่ ๖-๒๕๕-๖-๐๐๑๔
- ทะเบียนเลขที่ ๖-๒๕๕-๖-๐๐๑๕
- ทะเบียนเลขที่ ๖-๒๕๕-๖-๐๐๑๖
- ทะเบียนเลขที่ ๖-๒๕๕-๖-๐๐๑๗
- ทะเบียนเลขที่ ๖-๒๕๕-๖-๐๐๑๘
- ทะเบียนเลขที่ ๖-๒๕๕-๖-๐๐๑๙
- ทะเบียนเลขที่ ๖-๒๕๕-๖-๐๐๒๐
- ทะเบียนเลขที่ ๖-๒๕๕-๖-๐๐๒๑
- ทะเบียนเลขที่ ๖-๒๕๕-๖-๐๐๒๒
- ทะเบียนเลขที่ ๖-๒๕๕-๖-๐๐๒๓
- ทะเบียนเลขที่ ๖-๒๕๕-๖-๐๐๒๔
- ทะเบียนเลขที่ ๖-๒๕๕-๖-๐๐๒๕
- ทะเบียนเลขที่ ๖-๒๕๕-๖-๐๐๒๖
- ทะเบียนเลขที่ ๖-๒๕๕-๖-๐๐๒๗
- ทะเบียนเลขที่ ๖-๒๕๕-๖-๐๐๒๘
- ทะเบียนเลขที่ ๖-๒๕๕-๖-๐๐๒๙
- ทะเบียนเลขที่ ๖-๒๕๕-๖-๐๐๓๐
- ทะเบียนเลขที่ ๖-๒๕๕-๖-๐๐๓๑
- ทะเบียนเลขที่ ๖-๒๕๕-๖-๐๐๓๒
- ทะเบียนเลขที่ ๖-๒๕๕-๖-๐๐๓๓
- ทะเบียนเลขที่ ๖-๒๕๕-๖-๐๐๓๔
- ทะเบียนเลขที่ ๖-๒๕๕-๖-๐๐๓๕
- ทะเบียนเลขที่ ๖-๒๕๕-๖-๐๐๓๖
- ทะเบียนเลขที่ ๖-๒๕๕-๖-๐๐๓๗
- ทะเบียนเลขที่ ๖-๒๕๕-๖-๐๐๓๘
- ทะเบียนเลขที่ ๖-๒๕๕-๖-๐๐๓๙
- ทะเบียนเลขที่ ๖-๒๕๕-๖-๐๐๔๐
- ทะเบียนเลขที่ ๖-๒๕๕-๖-๐๐๔๑
- ทะเบียนเลขที่ ๖-๒๕๕-๖-๐๐๔๒
- ทะเบียนเลขที่ ๖-๒๕๕-๖-๐๐๔๓
- ทะเบียนเลขที่ ๖-๒๕๕-๖-๐๐๔๔
- ทะเบียนเลขที่ ๖-๒๕๕-๖-๐๐๔๕
- ทะเบียนเลขที่ ๖-๒๕๕-๖-๐๐๔๖
- ทะเบียนเลขที่ ๖-๒๕๕-๖-๐๐๔๗
- ทะเบียนเลขที่ ๖-๒๕๕-๖-๐๐๔๘
- ทะเบียนเลขที่ ๖-๒๕๕-๖-๐๐๔๙
- ทะเบียนเลขที่ ๖-๒๕๕-๖-๐๐๕๐
- ทะเบียนเลขที่ ๖-๒๕๕-๖-๐๐๕๑
- ทะเบียนเลขที่ ๖-๒๕๕-๖-๐๐๕๒
- ทะเบียนเลขที่ ๖-๒๕๕-๖-๐๐๕๓
- ทะเบียนเลขที่ ๖-๒๕๕-๖-๐๐๕๔
- ทะเบียนเลขที่ ๖-๒๕๕-๖-๐๐๕๕
- ทะเบียนเลขที่ ๖-๒๕๕-๖-๐๐๕๖
- ทะเบียนเลขที่ ๖-๒๕๕-๖-๐๐๕๗
- ทะเบียนเลขที่ ๖-๒๕๕-๖-๐๐๕๘

๓๙๖

๓๙๓) นางสาวบัณฑิต...

- ๓๙๓) นางสาวบัณฑิตา ชูเชิดเชื้อ
- ๓๙๔) นางสาวลลิตาวัลย์ โพธิ์พันธ์
- ๓๙๕) นายอาทิตย์ ตาภา
- ๓๙๖) นางสาวบุญยงพร บุญถนอมศรี
- ๓๙๗) นางสาวพัชรารัตน์ ชินธิบุตร
- ๓๙๘) นางสาวนฤกร ได้บ้านกวย
- ๓๙๙) นางสาวปวีณา แคนชบ
- ๔๐๐) นางสาวนันทิชา พรหมกัญญา
- ๔๐๑) นางสาวกมลชนก ปูนคำ
- ๔๐๒) นางสาวปวีณิดา ทองใบ
- ๔๐๓) นายชัยวัฒน์ ชินละคร
- ๔๐๔) นางสาวกัญญา สิงห์แก้ว
- ๔๐๕) นางสาวอารีนา มณีเชีย
- ๔๐๖) นายสุภาพกรณ์ อุนรา
- ๔๐๗) นางสาวชามันดา กิมาคม
- ๔๐๘) นายอนันต์นรินทร์ ยาเหลี่ยม
- ๔๐๙) นายวีระพงษ์ แสงทำนง
- ๔๑๐) นางสาวปิยะณัฐชา สำเภาพงษ์
- ๔๑๑) นางสาวนันทิสร ศรีสถาน
- ๔๑๒) นางสาวจุริวัณน์ โสแทน
- ๔๑๓) นายธีรวัฒน์ ทรงแลา
- ๔๑๔) นายอนันต์พงษ์ ปลั่งกลาง
- ๔๑๕) นายณภัทร เตยบุตร
- ๔๑๖) นางสาวจิตาภา ฤชา
- ๔๑๗) นางสาวณัฐชญาทิพย์ สังข์ทอง
- ๔๑๘) นางสาวชาริษา บาบุญ
- ๔๑๙) นายภูวดล เหมมา
- ๔๒๐) ว่าที่ร้อยตรีวิมลพร ประทุมเขตต์
- ๔๒๑) นายอนุทร พลสำโรง

- ทะเบียนเลขที่ ๖-๒๕๕-๖-๐๐๖๐
- ทะเบียนเลขที่ ๖-๒๕๕-๖-๐๐๖๑
- ทะเบียนเลขที่ ๖-๒๕๕-๖-๐๐๖๒
- ทะเบียนเลขที่ ๖-๒๕๕-๖-๐๐๖๓
- ทะเบียนเลขที่ ๖-๒๕๕-๖-๐๐๖๔
- ทะเบียนเลขที่ ๖-๒๕๕-๖-๐๐๖๕
- ทะเบียนเลขที่ ๖-๒๕๕-๖-๐๐๖๖
- ทะเบียนเลขที่ ๖-๒๕๕-๖-๐๐๖๗
- ทะเบียนเลขที่ ๖-๒๕๕-๖-๐๐๖๘
- ทะเบียนเลขที่ ๖-๒๕๕-๖-๐๐๖๙
- ทะเบียนเลขที่ ๖-๒๕๕-๖-๐๐๗๐
- ทะเบียนเลขที่ ๖-๒๕๕-๖-๐๐๗๑
- ทะเบียนเลขที่ ๖-๒๕๕-๖-๐๐๗๒
- ทะเบียนเลขที่ ๖-๒๕๕-๖-๐๐๗๓
- ทะเบียนเลขที่ ๖-๒๕๕-๖-๐๐๗๔
- ทะเบียนเลขที่ ๖-๒๕๕-๖-๐๐๗๕
- ทะเบียนเลขที่ ๖-๒๕๕-๖-๐๐๗๖
- ทะเบียนเลขที่ ๖-๒๕๕-๖-๐๐๗๗
- ทะเบียนเลขที่ ๖-๒๕๕-๖-๐๐๗๘
- ทะเบียนเลขที่ ๖-๒๕๕-๖-๐๐๗๙
- ทะเบียนเลขที่ ๖-๒๕๕-๖-๐๐๘๐
- ทะเบียนเลขที่ ๖-๒๕๕-๖-๐๐๘๑
- ทะเบียนเลขที่ ๖-๒๕๕-๖-๐๐๘๒
- ทะเบียนเลขที่ ๖-๒๕๕-๖-๐๐๘๓
- ทะเบียนเลขที่ ๖-๒๕๕-๖-๐๐๘๔
- ทะเบียนเลขที่ ๖-๒๕๕-๖-๐๐๘๕
- ทะเบียนเลขที่ ๖-๒๕๕-๖-๐๐๘๖
- ทะเบียนเลขที่ ๖-๒๕๕-๖-๐๐๘๗
- ทะเบียนเลขที่ ๖-๒๕๕-๖-๐๐๘๘
- ทะเบียนเลขที่ ๖-๒๕๕-๖-๐๐๘๙
- ทะเบียนเลขที่ ๖-๒๕๕-๖-๐๐๙๐
- ทะเบียนเลขที่ ๖-๒๕๕-๖-๐๐๙๑
- ทะเบียนเลขที่ ๖-๒๕๕-๖-๐๐๙๒
- ทะเบียนเลขที่ ๖-๒๕๕-๖-๐๐๙๓
- ทะเบียนเลขที่ ๖-๒๕๕-๖-๐๐๙๔
- ทะเบียนเลขที่ ๖-๒๕๕-๖-๐๐๙๕
- ทะเบียนเลขที่ ๖-๒๕๕-๖-๐๐๙๖
- ทะเบียนเลขที่ ๖-๒๕๕-๖-๐๐๙๗
- ทะเบียนเลขที่ ๖-๒๕๕-๖-๐๐๙๘
- ทะเบียนเลขที่ ๖-๒๕๕-๖-๐๐๙๙
- ทะเบียนเลขที่ ๖-๒๕๕-๖-๐๑๐๐

๓๙๖

๓๙๕) นายบัณฑิต...

เอกสารแนบท้ายหนังสือตอบรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน
บริษัท ยูไนเต็ด แอนาไลติก แอนด์ เอ็นจิเนียริ่ง คอนซัลแตนท์ จำกัด เลขทะเบียน ๖-๒๕๕
ที่ อก ๐๓๑๐(๑) ๖ ๐ ๘ ๕ ลงวันที่ ๐๗ กุมภาพันธ์ ๒๕๖๕

ขอขำสารมลพิษที่ได้รับขึ้นทะเบียนจากกรมโรงงานอุตสาหกรรม จำนวน ๓๗ รายการ

แนบท้าย จำนวน 46 รายการ

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
1	Aldrin	Liquid-Liquid Extraction, Gas Chromatographic Method ⁽¹⁾
2	Arsenic	1) Digestion, Hydride Generation/Atomic Absorption Spectrometric Method ⁽¹⁾ 2) Digestion, Inductively Coupled Plasma Method ⁽¹⁾
3	Barium	Digestion, Inductively Coupled Plasma Method ⁽¹⁾
4	α-BHC	Liquid-Liquid Extraction, Gas Chromatographic Method ⁽¹⁾
5	β-BHC	Liquid-Liquid Extraction, Gas Chromatographic Method ⁽¹⁾
6	δ-BHC	Liquid-Liquid Extraction, Gas Chromatographic Method ⁽¹⁾
7	γ-BHC	Liquid-Liquid Extraction, Gas Chromatographic Method ⁽¹⁾
8	Biochemical Oxygen Demand	1) 5-Day BOD Test, Azide Modification Method ⁽¹⁾ 2) 5-Day BOD Test, Membrane Electrode Method ⁽¹⁾
9	Cadmium	1) Digestion, Direct Air-Acetylene Flame Method ⁽¹⁾ 2) Digestion, Inductively Coupled Plasma Method ⁽¹⁾
10	Chemical Oxygen Demand	1) Closed Reflux, Titrimetric Method ⁽¹⁾ 2) Closed Reflux, Colorimetric Method ⁽¹⁾ 3) Open Reflux, Titrimetric Method ⁽¹⁾
11	Chlordane	Liquid-Liquid Extraction, Gas Chromatographic Method ⁽¹⁾
12	Chromium	1) Digestion, Direct Air-Acetylene Flame Method ⁽¹⁾ 2) Digestion, Inductively Coupled Plasma Method ⁽¹⁾
13	Color	ADMI Weighted-Ordinate Spectrophotometric Method ⁽¹⁾
14	Copper	1) Digestion, Direct Air-Acetylene Flame Method ⁽¹⁾ 2) Digestion, Inductively Coupled Plasma Method ⁽¹⁾
15	Cyanide	1) Distillation, Colorimetric Method ⁽¹⁾ 2) Total Cyanide after Distillation, by Flow Injection Analysis Method ⁽¹⁾
16	o,p'-DDT	Liquid-Liquid Extraction, Gas Chromatographic Method ⁽¹⁾
17	4,4'-DDD	Liquid-Liquid Extraction, Gas Chromatographic Method ⁽¹⁾
18	4,4'-DDE	Liquid-Liquid Extraction, Gas Chromatographic Method ⁽¹⁾
19	4,4'-DDT	Liquid-Liquid Extraction, Gas Chromatographic Method ⁽¹⁾
20	Dieldrin	Liquid-Liquid Extraction, Gas Chromatographic Method ⁽¹⁾
21	Endosulfan I	Liquid-Liquid Extraction, Gas Chromatographic Method ⁽¹⁾
22	Endosulfan II	Liquid-Liquid Extraction, Gas Chromatographic Method ⁽¹⁾
23	Endosulfan sulfate	Liquid-Liquid Extraction, Gas Chromatographic Method ⁽¹⁾
24	Endrin	Liquid-Liquid Extraction, Gas Chromatographic Method ⁽¹⁾

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
25	Endrin aldehyde	Liquid-Liquid Extraction, Gas Chromatographic Method ⁽⁴⁾
26	Formaldehyde	Distillation, Colorimetric Method ⁽²⁾
27	Free Chlorine	1) Iodometric Method ⁽⁴⁾ 2) DPD Ferrous Titrimetric Method ⁽⁴⁾
28	Heptachlor	Liquid-Liquid Extraction, Gas Chromatographic Method ⁽⁴⁾
29	Heptachlor Epoxide	Liquid-Liquid Extraction, Gas Chromatographic Method ⁽⁴⁾
30	Hexavalent Chromium	Colorimetric Method ⁽⁴⁾
31	Lead	1) Digestion, Direct Air-Acetylene Flame Method ⁽⁴⁾ 2) Digestion, Inductively Coupled Plasma Method ⁽⁴⁾
32	Manganese	1) Digestion, Direct Air-Acetylene Flame Method ⁽⁴⁾ 2) Digestion, Inductively Coupled Plasma Method ⁽⁴⁾
33	Mercury	Digestion, Cold-Vapor Atomic Absorption Spectrometric Method ⁽⁴⁾
34	Methoxychlor	Liquid-Liquid Extraction, Gas Chromatographic Method ⁽⁴⁾
35	Nickel	1) Digestion, Direct Air-Acetylene Flame Method ⁽⁴⁾ 2) Digestion, Inductively Coupled Plasma Method ⁽⁴⁾
36	Oil & Grease	1) Liquid-Liquid, Partition-Gravimetric Method ⁽⁴⁾ 2) Soxhlet Extraction Method ⁽⁴⁾
37	pH	Electrometric Method ⁽⁴⁾
38	Phenols	1) Distillation, Chloroform Extraction Method ⁽⁴⁾ 2) Distillation, Direct Photometric Method ⁽⁴⁾
39	Selenium	1) Digestion, Hydride Generation/Atomic Absorption Spectrometric Method ⁽⁴⁾ 2) Digestion, Inductively Coupled Plasma Method ⁽⁴⁾
40	Sulfide	1) Iodometric Method ⁽⁴⁾ 2) Methylene Blue Method ⁽⁴⁾
41	Temperature	Laboratory and Field Methods ⁽⁴⁾
42	Total Dissolved Solids	Dried at 180 °C ⁽⁴⁾
43	Total Kjeldahl Nitrogen	Semi-Micro-Kjeldahl Method ⁽⁴⁾
44	Total Suspended Solids	Dried from 103 to 105 °C ⁽⁴⁾
45	Trivalent Chromium	1) Digestion, Direct Air-Acetylene Flame Method; Colorimetric Method; Calculation ⁽⁴⁾ 2) Digestion, Inductively Coupled Plasma Method; Colorimetric Method; Calculation ⁽⁴⁾
46	Zinc	1) Digestion, Direct Air-Acetylene Flame Method ⁽⁴⁾ 2) Digestion, Inductively Coupled Plasma Method ⁽⁴⁾

น้ำใต้ดิน...

น้ำใต้ดิน จำนวน 126 รายการ

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
1	Acenaphthene	1) Liquid-Liquid Extraction, Gas Chromatographic Method ⁽⁴⁾
2	Acetone	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
3	Aldrin	1) Liquid-Liquid Extraction, Gas Chromatographic Method ⁽⁴⁾ 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
4	Anthracene	1) Liquid-Liquid Extraction, Gas Chromatographic Method ⁽⁴⁾ 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
5	Antimony	Digestion, Inductively Coupled Plasma Method ⁽⁴⁾
6	Arsenic	1) Digestion, Hydride Generation/Atomic Absorption Spectrometric Method ⁽⁴⁾ 2) Digestion, Inductively Coupled Plasma Method ⁽⁴⁾
7	Atrazine	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
8	Barium	Digestion, Inductively Coupled Plasma Method ⁽⁴⁾
9	Benz(a)anthracene	1) Liquid-Liquid Extraction, Gas Chromatographic Method ⁽⁴⁾ 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
10	Benzene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
11	Benzo(b)fluoranthene	1) Liquid-Liquid Extraction, Gas Chromatographic Method ⁽⁴⁾ 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
12	Benzo(k)fluoranthene	1) Liquid-Liquid Extraction, Gas Chromatographic Method ⁽⁴⁾ 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
13	Benzoic acid	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾

14 Benzo(a)pyrene...

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
14	Benzo(a)pyrene	1) Liquid-Liquid Extraction, Gas Chromatographic Method ⁽⁴⁾ 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
15	Benzo(g,h,i)perylene	1) Liquid-Liquid Extraction, Gas Chromatographic Method ⁽⁴⁾ 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
16	Beryllium	Digestion, Inductively Coupled Plasma Method ⁽⁴⁾
17	Bis(2-chloroethyl)ether	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
18	Bis(2-ethylhexyl)phthalate	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
19	Bromodichloromethane	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
20	Bromoform	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
21	Butanol	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
22	Butyl benzyl phthalate	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
23	Cadmium	1) Digestion, Direct Air-Acetylene Flame Method ⁽⁴⁾ 2) Digestion, Electrothermal Atomic Absorption Spectrometric Method ⁽⁴⁾ 3) Digestion, Inductively Coupled Plasma Method ⁽⁴⁾
24	Carbazole	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
25	Carbon disulfide	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
26	Carbon tetrachloride	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
27	Chlordane	1) Liquid-Liquid Extraction, Gas Chromatographic Method ⁽⁴⁾ 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
28	p-Chloroaniline	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾

29 Chlorobenzene...

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
29	Chlorobenzene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
30	Chlorodibromomethane	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
31	Chloroform	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
32	2-Chlorophenol	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
33	Chromium	1) Digestion, Direct Air-Acetylene Flame Method ⁽⁴⁾ 2) Digestion, Inductively Coupled Plasma Method ⁽⁴⁾
34	Chromium (III)	1) Digestion, Direct Air-Acetylene Flame Method; Colorimetric Method; Calculation ⁽⁴⁾ 2) Digestion, Inductively Coupled Plasma Method; Colorimetric Method; Calculation ⁽⁴⁾
35	Chromium (VI)	Colorimetric Method ⁽⁴⁾
36	Chrysene	1) Liquid-Liquid Extraction, Gas Chromatographic Method ⁽⁴⁾ 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
37	Cyanide	Distillation, Colorimetric Method ⁽⁴⁾
38	2,4-D	Liquid-Liquid Extraction, Gas Chromatographic Method ⁽⁴⁾
39	DDD	1) Liquid-Liquid Extraction, Gas Chromatographic Method ⁽⁴⁾ 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
40	DDE	1) Liquid-Liquid Extraction, Gas Chromatographic Method ⁽⁴⁾ 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
41	DDT	1) Liquid-Liquid Extraction, Gas Chromatographic Method ⁽⁴⁾ 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
42	Dibenz(a,h)anthracene	1) Liquid-Liquid Extraction, Gas Chromatographic Method ⁽⁴⁾ 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾

43 Di-n-butyl phthalate...

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
43	Di-n-butyl phthalate	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
44	1,2-Dichlorobenzene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
45	1,3-Dichlorobenzene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
46	1,4-Dichlorobenzene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
47	3,3'-Dichlorobenzidine	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
48	1,1-Dichloroethane	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
49	1,2-Dichloroethane	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
50	1,1-Dichloroethylene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
51	cis-1,2-Dichloroethylene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
52	trans-1,2-Dichloroethylene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
53	2,4-Dichlorophenol	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
54	1,2-Dichloropropane	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
55	1,3-Dichloropropane	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
56	1,3-Dichloropropene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
57	Dieldrin	1) Liquid-Liquid Extraction, Gas Chromatographic Method ⁽⁴⁾ 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
58	Diethyl phthalate	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
59	2,4-Dimethylphenol	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
60	2,4-Dinitrophenol	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾

61 2,4-Dinitrotoluene...

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
61	2,4-Dinitrotoluene	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
62	2,6-Dinitrotoluene	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
63	Di-n-Octyl phthalate	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
64	Endosulfan	1) Liquid-Liquid Extraction, Gas Chromatographic Method ⁽⁴⁾ 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
65	Endrin	1) Liquid-Liquid Extraction, Gas Chromatographic Method ⁽⁴⁾ 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
66	Ethylbenzene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
67	Fluoranthene	1) Liquid-Liquid Extraction, Gas Chromatographic Method ⁽⁴⁾ 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
68	Fluorene	1) Liquid-Liquid Extraction, Gas Chromatographic Method ⁽⁴⁾ 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
69	Heptachlor	1) Liquid-Liquid Extraction, Gas Chromatographic Method ⁽⁴⁾ 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
70	Heptachlor epoxide	1) Liquid-Liquid Extraction, Gas Chromatographic Method ⁽⁴⁾ 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
71	Hexachlorobenzene	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
72	Hexachloro-1,3-butadiene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
73	n-Hexane	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾

74 α -HCH...

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
74	α -HCH	1) Liquid-Liquid Extraction, Gas Chromatographic Method ⁽⁴⁾ 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
75	β -HCH	1) Liquid-Liquid Extraction, Gas Chromatographic Method ⁽⁴⁾ 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
76	γ -HCH	1) Liquid-Liquid Extraction, Gas Chromatographic Method ⁽⁴⁾ 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
77	Hexachlorocyclopentadiene	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
78	Hexachloroethane	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
79	Indeno(1,2,3-cd)pyrene	1) Liquid-Liquid Extraction, Gas Chromatographic Method ⁽⁴⁾ 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
80	Isophorone	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
81	Lead	1) Digestion, Direct Air-Acetylene Flame Method ⁽⁴⁾ 2) Digestion, Electrothermal Atomic Absorption Spectrometric Method ⁽⁴⁾ 3) Digestion, Inductively Coupled Plasma Method ⁽⁴⁾
82	Manganese	1) Digestion, Direct Air-Acetylene Flame Method ⁽⁴⁾ 2) Digestion, Inductively Coupled Plasma Method ⁽⁴⁾
83	Mercury	Digestion, Cold-Vapor Atomic Absorption Spectrometric Method ⁽⁴⁾
84	Methanol	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
85	Methoxychlor	1) Liquid-Liquid Extraction, Gas Chromatographic Method ⁽⁴⁾ 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
86	Methyl bromide	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾

87 Methylene chloride...

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
87	Methylene chloride	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
88	2-Methylphenol	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
89	2-Methylnaphthalene	1) Liquid-Liquid Extraction, Gas Chromatographic Method ⁽⁴⁾ 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
90	Methyl tert-butyl ether	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
91	Naphthalene	1) Liquid-Liquid Extraction, Gas Chromatographic Method ⁽⁴⁾ 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
92	Nickel	1) Digestion, Direct Air-Acetylene Flame Method ⁽⁴⁾ 2) Digestion, Inductively Coupled Plasma Method ⁽⁴⁾
93	Nitrobenzene	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
94	N-Nitrosodiphenylamine	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
95	N-Nitrosodi-n-propylamine	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
96	Polychlorinated Biphenyls - PCB 1016 - PCB 1221 - PCB 1232 - PCB 1242 - PCB-1248 - PCB-1254 - PCB-1260	1) Liquid-Liquid Extraction, Gas Chromatographic Method ⁽⁴⁾ 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
97	Pentachlorophenol	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
98	pH	Electrometric Method ⁽⁴⁾
99	Phenanthrene	1) Liquid-Liquid Extraction, Gas Chromatographic Method ⁽⁴⁾ 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾

100 Phenol...

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
100	Phenol	1) Distillation, Chloroform Extraction Method ⁽⁴⁾ 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
101	Pyrene	1) Liquid-Liquid Extraction, Gas Chromatographic Method ⁽⁴⁾ 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
102	Selenium	1) Digestion, Hydride Generation/Atomic Absorption Spectrometric Method ⁽⁴⁾ 2) Digestion, Inductively Coupled Plasma Method ⁽⁴⁾
103	Silver	Digestion, Inductively Coupled Plasma Method ⁽⁴⁾
104	Styrene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
105	1,1,2,2-Tetrachloroethane	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
106	Tetrachloroethylene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
107	Toluene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
108	Toxaphene	1) Liquid-Liquid Extraction, Gas Chromatographic Method ⁽⁴⁾ 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
109	TPH (C ₃ - C ₆)	1) Purge and Trap, Gas Chromatographic Method ^(12,22) 2) Purge and Trap, Gas Chromatographic/Mass spectrometric Method ^(12,27)
110	TPH (C ₈ - C ₁₆)	Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method ^(9,22)
111	TPH (C ₁₆ - C ₃₅)	Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method ^(9,22)
112	1,2,4-Trichlorobenzene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
113	1,1,1-Trichloroethane	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
114	1,1,2-Trichloroethane	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
115	Trichloroethylene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾

116 2,4,5-Trichlorophenol...

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
116	2,4,5-Trichlorophenol	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
117	2,4,6-Trichlorophenol	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
118	1,3,5-Trimethylbenzene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
119	Vanadium	Digestion, Inductively Coupled Plasma Method ⁽⁴⁾
120	Vinyl acetate	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
121	Vinyl chloride	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
122	m-Xylene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
123	o-Xylene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
124	p-Xylene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
125	Xylene (Total)	Purge and Trap Gas Chromatographic/Mass Spectrometric Method ⁽⁴⁾
126	Zinc	1) Digestion, Direct Air-Acetylene Flame Method ⁽⁴⁾ 2) Digestion, Inductively Coupled Plasma Method ⁽⁴⁾

ตารางสืบ (ปล่องระบาย) จำนวน 25 รายการ

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
1	Antimony	Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method ⁽⁵⁾
2	Arsenic	1) Isokinetic Sampling, Digestion, Hydride Generation/Atomic Absorption Spectrometric Method ⁽⁵⁾ 2) Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method ⁽⁵⁾
3	Cadmium	1) Isokinetic Sampling, Digestion, Direct Air-Acetylene Flame Method ⁽⁵⁾ 2) Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method ⁽⁵⁾
4	Carbon Monoxide	Instrumental Analyzer Method ⁽⁵⁾
5	Chlorine	Isokinetic Sampling, Ion Chromatographic Method ⁽⁵⁾
6	Chromium	1) Isokinetic Sampling, Digestion, Direct Air-Acetylene Flame Method ⁽⁵⁾

Chromium (ต่อ)...

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
6	Chromium (ต่อ)	2) Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method ⁽⁵⁾
7	Cobalt	Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method ⁽⁵⁾
8	Copper	1) Isokinetic Sampling, Digestion, Direct Air-Acetylene Flame Method ⁽⁵⁾ 2) Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method ⁽⁵⁾
9	Cresol	Absorption Sampling, Gas Chromatographic Method ⁽⁵⁾
10	Dioxins/Furans	Isokinetic Sampling ⁽⁵⁾
11	Hydrogen Chloride	Isokinetic Sampling, Ion Chromatographic Method ⁽⁵⁾
12	Hydrogen Fluoride	Isokinetic Sampling, Ion Chromatographic Method ⁽⁵⁾
13	Hydrogen Sulfide	Absorption Sampling, Iodometric Method ⁽⁵⁾
14	Lead	1) Isokinetic Sampling, Digestion, Direct Air-Acetylene Flame Method ⁽⁵⁾ 2) Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method ⁽⁵⁾
15	Manganese	1) Isokinetic Sampling, Digestion, Direct Air-Acetylene Flame Method ⁽⁵⁾ 2) Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method ⁽⁵⁾
16	Mercury	Isokinetic Sampling, Digestion, Cold-Vapor Atomic Absorption Spectrometric Method ⁽⁵⁾
17	Nickel	1) Isokinetic Sampling, Digestion, Direct Air-Acetylene Flame Method ⁽⁵⁾ 2) Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method ⁽⁵⁾
18	Opacity	Ringelmann's Method ⁽¹⁾
19	Oxides of Nitrogen	1) Absorption Sampling, Phenoldisulfonic acid Method ⁽⁵⁾ 2) Instrumental Analyzer Method ⁽⁵⁾
20	Selenium	1) Isokinetic Sampling, Digestion, Hydride Generation/Atomic Absorption Spectrometric Method ⁽⁵⁾ 2) Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method ⁽⁵⁾
21	Sulfur Dioxide	1) Absorption Sampling, Barium-Thorin Titrimetric Method ⁽⁵⁾ 2) Instrumental Analyzer Method ⁽⁵⁾
22	Sulfuric Acid	Isokinetic Sampling, Barium-Thorin Titrimetric Method ⁽⁵⁾

23 Total Suspended Particulate...

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
23	Total Suspended Particulate	Isokinetic Sampling, Gravimetric Method ⁽⁵⁾
24	Vanadium	Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method ⁽⁵⁾
25	Xylene	1) Bag Sampling, Gas Chromatographic Method ⁽⁵⁾ 2) Adsorption Sampling, Gas Chromatographic Method ⁽⁵⁾

สิ่งปนเปื้อนหรือวัสดุที่ไม่ใช่แล้ว จำนวน 35 รายการ

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
1	Aldrin	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method ^(3,9,23) 2) Ultrasonic Extraction, Gas Chromatographic Method ^(10,23)
2	Antimony	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^(3,6,14) 2) Digestion, Inductively Coupled Plasma Method ^(7,14)
3	Arsenic	1) Waste Extraction, Digestion, Hydride Generation/Atomic Absorption Spectrometric Method ^(3,6,14) 2) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^(3,6,14) 3) Digestion, Hydride Generation/Atomic Absorption Spectrometric Method ^(7,14) 4) Digestion, Inductively Coupled Plasma Method ^(7,14)
4	Barium	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^(3,6,14) 2) Digestion, Inductively Coupled Plasma Method ^(7,14)
5	Beryllium	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^(3,6,14) 2) Digestion, Inductively Coupled Plasma Method ^(7,14)
6	Cadmium	1) Waste Extraction, Digestion, Flame Atomic Absorption Spectrometric Method ^(3,6,15) 2) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^(3,6,14) 3) Digestion, Flame Atomic Absorption Spectrometric Method ^(7,15) 4) Digestion, Inductively Coupled Plasma Method ^(7,14)
7	Chlordane	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method ^(3,9,23) 2) Ultrasonic Extraction, Gas Chromatographic Method ^(10,23)

8 Chromium...

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
8	Chromium	1) Waste Extraction, Digestion, Flame Atomic Absorption Spectrometric Method ^(3,6,13) 2) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^(3,6,14) 3) Digestion, Flame Atomic Absorption Spectrometric Method ^(7,15) 4) Digestion, Inductively Coupled Plasma Method ^(7,14)
9	Chromium (III)	1) Waste Extraction, Digestion, Flame Atomic Absorption Spectrometric Method; Waste Extraction, Colorimetric Method; Calculation ^(3,6,15,17) 2) Waste Extraction, Digestion, Inductively Coupled Plasma Method; Waste Extraction, Colorimetric Method; Calculation ^(3,6,14,17) 3) Digestion, Flame Atomic Absorption Spectrometric Method; Alkaline Digestion, Colorimetric Method; Calculation ^(7,8,15,17) 4) Digestion, Inductively Coupled Plasma Method; Alkaline Digestion, Colorimetric Method; Calculation ^(7,8,14,17)
10	Chromium (VI)	1) Waste Extraction, Colorimetric Method ^(3,17) 2) Alkaline Digestion, Colorimetric Method ^(8,17)
11	Cobalt	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^(3,6,14) 2) Digestion, Inductively Coupled Plasma Method ^(7,14)
12	Copper	1) Waste Extraction, Digestion, Flame Atomic Absorption Spectrometric Method ^(3,6,13) 2) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^(3,6,14) 3) Digestion, Flame Atomic Absorption Spectrometric Method ^(7,15) 4) Digestion, Inductively Coupled Plasma Method ^(7,14)
13	2,4-D	1) Waste Extraction, Gas Chromatographic Method ^(3,26) 2) Ultrasonic Extraction, Gas Chromatographic Method ⁽²⁶⁾
14	DDD	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method ^(3,9,23) 2) Ultrasonic Extraction, Gas Chromatographic Method ^(10,23)

15 DDE...

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
15	DDE	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method ^(3,9,23) 2) Ultrasonic Extraction, Gas Chromatographic Method ^(10,23)
16	DDT	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method ^(3,9,23) 2) Ultrasonic Extraction, Gas Chromatographic Method ^(10,23)
17	Dieldrin	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method ^(3,9,23) 2) Ultrasonic Extraction, Gas Chromatographic Method ^(10,23)
18	Endrin	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method ^(3,9,23) 2) Ultrasonic Extraction, Gas Chromatographic Method ^(10,23)
19	Heptachlor	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method ^(3,9,23) 2) Ultrasonic Extraction, Gas Chromatographic Method ^(10,23)
20	Lead	1) Waste Extraction, Digestion, Flame Atomic Absorption Spectrometric Method ^(3,6,13) 2) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^(3,6,14) 3) Digestion, Flame Atomic Absorption Spectrometric Method ^(7,15) 4) Digestion, Inductively Coupled Plasma Method ^(7,14)
21	Lindane	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method ^(3,9,23) 2) Ultrasonic Extraction, Gas Chromatographic Method ^(10,23)
22	Mercury	1) Waste Extraction, Digestion, Cold-Vapor Atomic Absorption Spectrometric Method ^(3,19) 2) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^(3,6,14) 3) Digestion, Cold-Vapor Atomic Absorption Spectrometric Method ⁽⁹⁾ 4) Digestion, Inductively Coupled Plasma Method ^(7,14)

Mercury (II)...

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
22	Mercury (ดีไอ)	5) Thermal Decomposition Amalgamation and Atomic Absorption Spectrometric Method ⁽²⁰⁾
23	Methoxychlor	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method ^(3,9,23) 2) Ultrasonic Extraction, Gas Chromatographic Method ^(10,23)
24	Molybdenum	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^(3,6,14) 2) Digestion, Inductively Coupled Plasma Method ^(7,14)
25	Nickel	1) Waste Extraction, Digestion, Flame Atomic Absorption Spectrometric Method ^(3,6,13) 2) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^(3,6,14) 3) Digestion, Flame Atomic Absorption Spectrometric Method ^(7,15) 4) Digestion, Inductively Coupled Plasma Method ^(7,14)
26	Polychlorinated Biphenyls - Aroclor 1016 - Aroclor 1221 - Aroclor 1232 - Aroclor 1242 - Aroclor 1248 - Aroclor 1254 - Aroclor 1260 - 2-Chlorobiphenyl - 2,3-Dichlorobiphenyl - 2,2',5'-Trichlorobiphenyl - 2,4',5'-Trichlorobiphenyl - 2,2',3,5'-Tetrachlorobiphenyl - 2,2',5,5'-Tetrachlorobiphenyl - 2,3',4,4'-Tetrachlorobiphenyl - 2,2',3,4,5'- Pentachlorobiphenyl - 2,2',4,5,5'- Pentachlorobiphenyl - 2,3,3',4,6- Pentachlorobiphenyl	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method ^(3,9,24) 2) Ultrasonic Extraction, Gas Chromatographic Method ^(10,26)

Polychlorinated Biphenyls(II)...

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
	Polychlorinated Biphenyls(ดีไอ) - 2,2',3,4,4',5'- Hexachlorobiphenyl - 2,2',3,4,5,5'- Hexachlorobiphenyl - 2,2',3,5,5',6- Hexachlorobiphenyl - 2,2',4,4',5,5'- Hexachlorobiphenyl - 2,2',3,3',4,4',5- Heptachlorobiphenyl - 2,2',3,4,4',5,5'- Heptachlorobiphenyl - 2,2',3,4',5,5',6- Heptachlorobiphenyl - 2,2',3,3',4,4',5,5',6- Nonachlorobiphenyl	
27	Pentachlorophenol	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^(3,9,28) 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^(10,28)
28	pH	Electrometric Method ^(31,32)
29	Selenium	1) Waste Extraction, Digestion, Hydride Generation/Atomic Absorption Spectrometric Method ^(3,6,21) 2) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^(3,6,14) 3) Digestion, Hydride Generation/Atomic Absorption Spectrometric Method ^(7,21) 4) Digestion, Inductively Coupled Plasma Method ^(7,14)
30	Silver	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^(3,6,14) 2) Digestion, Inductively Coupled Plasma Method ^(7,14)
31	Thallium	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^(3,6,14) 2) Digestion, Inductively Coupled Plasma Method ^(7,14)

32 Toxaphene...

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
32	Toxaphene	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method ^(3,9,23) 2) Ultrasonic Extraction, Gas Chromatographic Method ^(10,23)
33	Trichloroethylene	1) Waste Extraction, Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^(3,11,27) 2) Waste Extraction, Equilibrium Headspace, Gas Chromatographic/Mass Spectrometric Method ^(3,11,27) 3) Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^(13,27) 4) Equilibrium Headspace, Gas Chromatographic/Mass Spectrometric Method ^(11,27)
34	Vanadium	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^(3,6,14) 2) Digestion, Inductively Coupled Plasma Method ^(7,14)
35	Zinc	1) Waste Extraction, Digestion, Flame Atomic Absorption Spectrometric Method ^(3,6,15) 2) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^(3,6,14) 3) Digestion, Flame Atomic Absorption Spectrometric Method ^(7,15) 4) Digestion, Inductively Coupled Plasma Method ^(7,14)

สิ้น จำนวน 125 รายการ

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
1	Acenaphthene	1) Ultrasonic Extraction, Gas Chromatographic Method ^(10,25) 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^(10,28)
2	Acetone	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^(13,27)
3	Aldrin	1) Ultrasonic Extraction, Gas Chromatographic Method ^(10,23) 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^(10,28)
4	Anthracene	1) Ultrasonic Extraction, Gas Chromatographic Method ^(10,25)

Anthracene (ตบ)..

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
4	Anthracene (ตบ)	2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^(10,28)
5	Antimony	Digestion, Inductively Coupled Plasma Method ^(7,14)
6	Arsenic	1) Digestion, Hydride Generation/Atomic Absorption Spectrometric Method ^(7,14) 2) Digestion, Inductively Coupled Plasma Method ^(7,14)
7	Atrazine	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^(10,28)
8	Barium	Digestion, Inductively Coupled Plasma Method ^(7,14)
9	Benz(a)anthracene	1) Ultrasonic Extraction, Gas Chromatographic Method ^(10,25) 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^(10,28)
10	Benzene	1) Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^(13,27) 2) Equilibrium Headspace, Gas Chromatographic/Mass Spectrometric Method ^(11,27)
11	Benzo(b)fluoranthene	1) Ultrasonic Extraction, Gas Chromatographic Method ^(10,25) 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^(10,28)
12	Benzo(k)fluoranthene	1) Ultrasonic Extraction, Gas Chromatographic Method ^(10,25) 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^(10,28)
13	Benzoic acid	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^(10,28)
14	Benzo(a)pyrene	1) Ultrasonic Extraction, Gas Chromatographic Method ^(10,25) 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^(10,28)
15	Benzo(g,h,i)perylene	1) Ultrasonic Extraction, Gas Chromatographic Method ^(10,25) 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^(10,28)
16	Beryllium	Digestion, Inductively Coupled Plasma Method ^(7,14)

17 Bis(2-chloroethyl)ether...

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
17	Bis(2-chloroethyl)ether	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^(10,28)
18	Bis(2-ethylhexyl)phthalate	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^(10,28)
19	Bromodichloromethane	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^(13,27)
20	Bromoform	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^(13,27)
21	Butanol	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^(13,27)
22	Butyl benzyl phthalate	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^(10,28)
23	Cadmium	1) Digestion, Flame Atomic Absorption Spectrometric Method ^(7,15) 2) Digestion, Inductively Coupled Plasma Method ^(7,14)
24	Carbazole	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^(10,28)
25	Carbon disulfide	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^(13,27)
26	Carbon tetrachloride	1) Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^(13,27) 2) Equilibrium Headspace, Gas Chromatographic/Mass Spectrometric Method ^(11,27)
27	Chlordane	1) Ultrasonic Extraction, Gas Chromatographic Method ^(10,25) 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^(10,28)
28	p-Chloroaniline	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^(10,28)
29	Chlorobenzene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^(13,27)
30	Chlorodibromomethane	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^(13,27)
31	Chloroform	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^(13,27)
32	2-Chlorophenol	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^(10,28)

33 Chromium...

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
33	Chromium	1) Digestion, Flame Atomic Absorption Spectrometric Method ^(7,15) 2) Digestion, Inductively Coupled Plasma Method ^(7,14)
34	Chromium (III)	1) Digestion, Flame Atomic Absorption Spectrometric Method; Alkaline Digestion, Colorimetric Method; Calculation ^(7,8,15,17) 2) Digestion, Inductively Coupled Plasma Method; Alkaline Digestion, Colorimetric Method; Calculation ^(7,8,14,17)
35	Chromium (VI)	Alkaline Digestion, Colorimetric Method ^(8,17)
36	Chrysene	1) Ultrasonic Extraction, Gas Chromatographic Method ^(10,25) 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^(10,28)
37	Cyanide	Extraction, Distillation, Colorimetric Method ^(29,30)
38	2,4-D	Ultrasonic Extraction, Gas Chromatographic Method ⁽²⁴⁾
39	DDD	1) Ultrasonic Extraction, Gas Chromatographic Method ^(10,23) 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^(10,28)
40	DOE	1) Ultrasonic Extraction, Gas Chromatographic Method ^(10,23) 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^(10,28)
41	DDT	1) Ultrasonic Extraction, Gas Chromatographic Method ^(10,23) 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^(10,28)
42	Dibenz(a,h)anthracene	1) Ultrasonic Extraction, Gas Chromatographic Method ^(10,25) 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^(10,28)
43	Di-n-butyl phthalate	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^(10,28)
44	1,2-Dichlorobenzene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^(13,27)

45 1,3-Dichlorobenzene...

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
45	1,3-Dichlorobenzene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^(13,27)
46	1,4-Dichlorobenzene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^(13,27)
47	3,3'-Dichlorobenzidine	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^(10,28)
48	1,1-Dichloroethane	1) Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^(13,27) 2) Equilibrium Headspace, Gas Chromatographic/Mass Spectrometric Method ^(11,27)
49	1,2-Dichloroethane	1) Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^(13,27) 2) Equilibrium Headspace, Gas Chromatographic/Mass Spectrometric Method ^(11,27)
50	1,1-Dichloroethylene	1) Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^(13,27) 2) Equilibrium Headspace, Gas Chromatographic/Mass Spectrometric Method ^(11,27)
51	cis-1,2-Dichloroethylene	1) Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^(13,27) 2) Equilibrium Headspace, Gas Chromatographic/Mass Spectrometric Method ^(11,27)
52	trans-1,2-Dichloroethylene	1) Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^(13,27) 2) Equilibrium Headspace, Gas Chromatographic/Mass Spectrometric Method ^(11,27)
53	2,4-Dichlorophenol	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^(10,28)
54	1,2-Dichloropropane	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^(13,27)
55	1,3-Dichloropropane	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^(13,27)
56	1,3-Dichloropropene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^(13,27)
57	Dieldrin	1) Ultrasonic Extraction, Gas Chromatographic Method ^(10,25) 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^(10,28)

58 Diethyl phthalate...

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
58	Diethyl phthalate	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^(10,28)
59	2,4-Dimethylphenol	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^(10,28)
60	2,4-Dinitrophenol	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^(10,28)
61	2,4-Dinitrotoluene	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^(10,28)
62	2,6-Dinitrotoluene	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^(10,28)
63	Di-n-Octyl phthalate	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^(10,28)
64	Endosulfan	1) Ultrasonic Extraction, Gas Chromatographic Method ^(10,25) 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^(10,28)
65	Endrin	1) Ultrasonic Extraction, Gas Chromatographic Method ^(10,25) 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^(10,28)
66	Ethylbenzene	1) Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^(13,27) 2) Equilibrium Headspace, Gas Chromatographic/Mass Spectrometric Method ^(11,27)
67	Fluoranthene	1) Ultrasonic Extraction, Gas Chromatographic Method ^(10,25) 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^(10,28)
68	Fluorene	1) Ultrasonic Extraction, Gas Chromatographic Method ^(10,25) 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^(10,28)
69	Heptachlor	1) Ultrasonic Extraction, Gas Chromatographic Method ^(10,25) 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^(10,28)
70	Heptachlor epoxide	1) Ultrasonic Extraction, Gas Chromatographic Method ^(10,25)

Heptachlor epoxide (พีบี)...

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
70	Heptachlor epoxide (พีบี)	2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^(10,28)
71	Hexachlorobenzene	1) Ultrasonic Extraction, Gas Chromatographic Method ^(10,25) 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^(10,28)
72	Hexachloro-1,3-butadiene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^(13,27)
73	n-Hexane	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^(13,27)
74	α-HCH	1) Ultrasonic Extraction, Gas Chromatographic Method ^(10,25) 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^(10,28)
75	β-HCH	1) Ultrasonic Extraction, Gas Chromatographic Method ^(10,25) 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^(10,28)
76	γ-HCH	1) Ultrasonic Extraction, Gas Chromatographic Method ^(10,25) 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^(10,28)
77	Hexachlorocyclopentadiene	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^(10,28)
78	Hexachloroethane	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^(10,28)
79	Indeno(1,2,3-cd)pyrene	1) Ultrasonic Extraction, Gas Chromatographic Method ^(10,25) 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^(10,28)
80	Isophorone	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^(10,28)
81	Lead	1) Digestion, Flame Atomic Absorption Spectrometric Method ^(7,15) 2) Digestion, Inductively Coupled Plasma Method ^(7,14)
82	Manganese	1) Digestion, Flame Atomic Absorption Spectrometric Method ^(7,15) 2) Digestion, Inductively Coupled Plasma Method ^(7,14)

83 Mercury...

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
83	Mercury	1) Digestion, Cold-Vapor Atomic Absorption Spectrometric Method ⁽⁹⁾ 2) Thermal Decomposition Amalgamation and Atomic Absorption Spectrometric Method ⁽²⁰⁾
84	Methanol	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^(13,27)
85	Methoxychlor	1) Ultrasonic Extraction, Gas Chromatographic Method ^(10,25) 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^(10,28)
86	Methyl bromide	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^(13,27)
87	Methylene chloride	1) Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^(13,27) 2) Equilibrium Headspace, Gas Chromatographic/Mass Spectrometric Method ^(11,27)
88	2-Methylphenol	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^(10,28)
89	2-Methylnaphthalene	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^(10,28)
90	Methyl tert-butyl ether	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^(13,27)
91	Naphthalene	1) Ultrasonic Extraction, Gas Chromatographic Method ^(10,25) 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^(10,28)
92	Nickel	1) Digestion, Flame Atomic Absorption Spectrometric Method ^(7,15) 2) Digestion, Inductively Coupled Plasma Method ^(7,14)
93	Nitrobenzene	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^(10,28)
94	N-Nitrosodiphenylamine	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^(10,28)
95	N-Nitrosodi-n-propylamine	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^(10,28)
96	Polychlorinated Biphenyls - Aroclor 1016	1) Ultrasonic Extraction, Gas Chromatographic Method ^(10,25)

Polychlorinated Biphenyls(พีบี)...

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
96	Polychlorinated Biphenyls(คอป) - Aroclor 1221 - Aroclor 1232 - Aroclor 1242 - Aroclor 1248 - Aroclor 1254 - Aroclor 1260 Polychlorinated Biphenyls - 2-Chlorobiphenyl - 2,3-Dichlorobiphenyl - 2,2',5-Trichlorobiphenyl - 2,4',5-Trichlorobiphenyl - 2,2',3,5'-Tetrachlorobiphenyl - 2,2',5,5'-Tetrachlorobiphenyl - 2,3',4,4'-Tetrachlorobiphenyl - 2,2',3,4,5'- Pentachlorobiphenyl - 2,2',4,5,5'- Pentachlorobiphenyl - 2,3,3',4',6- Pentachlorobiphenyl - 2,2',3,4,4',5'- Hexachlorobiphenyl - 2,2',3,4,5,5'- Hexachlorobiphenyl - 2,2',3,5,5',6- Hexachlorobiphenyl - 2,2',4,4',5,5'- Hexachlorobiphenyl - 2,2',3,3',4,4',5- Heptachlorobiphenyl - 2,2',3,4,4',5,5'- Heptachlorobiphenyl - 2,2',3,4,4',5,6- Heptachlorobiphenyl - 2,2',3,4',5,5',6- Heptachlorobiphenyl - 2,2',3,3',4,4',5,5',6- Nonachlorobiphenyl	2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^(10,20) Ultrasonic Extraction, Gas Chromatographic Method ^(10,20)

97 Pentachlorophenol...

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
97	Pentachlorophenol	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^(10,20)
98	Phenanthrene	1) Ultrasonic Extraction, Gas Chromatographic Method ^(10,25) 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^(10,20)
99	Phenol	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^(10,20)
100	Pyrene	1) Ultrasonic Extraction, Gas Chromatographic Method ^(10,25) 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^(10,20)
101	Selenium	1) Digestion, Hydride Generation/Atomic Absorption Spectrometric Method ^(7,21) 2) Digestion, Inductively Coupled Plasma Method ^(7,14)
102	Silver	Digestion, Inductively Coupled Plasma Method ^(7,14)
103	Styrene	1) Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^(13,27) 2) Equilibrium Headspace, Gas Chromatographic/Mass Spectrometric Method ^(13,27)
104	1,1,2,2-Tetrachloroethane	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^(13,27)
105	Tetrachloroethylene	1) Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^(13,27) 2) Equilibrium Headspace, Gas Chromatographic/Mass Spectrometric Method ^(13,27)
106	Toluene	1) Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^(13,27) 2) Equilibrium Headspace, Gas Chromatographic/Mass Spectrometric Method ^(13,27)
107	Toxaphene	Ultrasonic Extraction, Gas Chromatographic Method ^(10,23)
108	TPH (C ₅ -C ₆)	1) Purge and Trap, Gas Chromatographic Method ^(13,27) 2) Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^(13,27)
109	TPH (C ₇ -C ₁₆)	Ultrasonic Extraction, Gas Chromatographic Method ^(10,22)
110	TPH (C _{>16} -C ₃₃)	Ultrasonic Extraction, Gas Chromatographic Method ^(10,22)

111 1,2,4-Trichlorobenzene...

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
111	1,2,4-Trichlorobenzene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^(13,27)
112	1,1,1-Trichloroethane	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^(13,27)
113	1,1,2-Trichloroethane	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^(13,27)
114	Trichloroethylene	1) Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^(13,27) 2) Equilibrium Headspace, Gas Chromatographic/Mass Spectrometric Method ^(11,27)
115	2,4,5-Trichlorophenol	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^(10,20)
116	2,4,6-Trichlorophenol	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^(10,20)
117	1,3,5-Trimethylbenzene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^(13,27)
118	Vanadium	Digestion, Inductively Coupled Plasma Method ^(7,14)
119	Vinyl acetate	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^(13,27)
120	Vinyl chloride	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^(13,27)
121	m-Xylene	1) Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^(13,27) 2) Equilibrium Headspace, Gas Chromatographic/Mass Spectrometric Method ^(11,27)
122	o-Xylene	1) Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^(13,27) 2) Equilibrium Headspace, Gas Chromatographic/Mass Spectrometric Method ^(11,27)
123	p-Xylene	1) Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^(13,27) 2) Equilibrium Headspace, Gas Chromatographic/Mass Spectrometric Method ^(11,27)
124	Xylene (Total)	1) Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^(13,27) 2) Equilibrium Headspace, Gas Chromatographic/Mass Spectrometric Method ^(11,27)

125 Zinc...

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
125	Zinc	1) Digestion, Flame Atomic Absorption Spectrometric Method ^(7,15) 2) Digestion, Inductively Coupled Plasma Method ^(7,14)

เอกสารอ้างอิง

- กระทรวงอุตสาหกรรม, ประกาศกระทรวงอุตสาหกรรม, พ.ศ. 2549. เรื่อง กำหนดค่าปริมาณมาตรฐานที่เจือปนในอากาศที่ระบายออกจากปล่องของหม้อน้ำโรงสีข้าวที่ใช้ถ่านหินเชื้อเพลิง. ราชกิจจานุเบกษา. 4 ธันวาคม 2549. เล่มที่ 123 ตอนพิเศษ 125จ.
- สมาคมวิศวกรรมสิ่งแวดล้อมแห่งประเทศไทย. คู่มือวิเคราะห์น้ำเสีย. พิมพ์ครั้งที่ 4. กรุงเทพฯ: เรือนแก้วการพิมพ์, 2547.
- กระทรวงอุตสาหกรรม, ประกาศกระทรวงอุตสาหกรรม, พ.ศ. 2566. เรื่อง การจัดการสิ่งปฏิกูลหรือวัสดุที่ไม่ใช้แล้ว ราชกิจจานุเบกษา. 31 พฤษภาคม 2566. เล่มที่ 140 ตอนพิเศษ 126 จ.
- APHA, AWWA, WEF. Standard Methods for the Examination of Water and Wastewater. 24th ed. Washington, DC: APHA, 2023.
- United States Environmental Protection Agency. Standards of Performance for New Stationary Sources. 40 CFR 60. Appendix A, 2020.
- United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. SW-846, 2014.
- United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. Acid Digestion of Sediments, Sludges, and Soils. SW-846 Method 3050B, 1996.
- United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. Alkaline Digestion for Hexavalent Chromium. SW-846 Method 3060A, 1996.
- United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste 3. Physical/Chemical Methods. Separatory Funnel Liquid-Liquid Extraction. SW-846 Method 3510C, 1996.
- United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. Ultrasonic Extraction. SW-846 Method 3550C, 2007.
- United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. Volatile Organic Compounds in Various Sample Matrices Using Equilibrium Headspace Analysis. SW-846 Method 5021A, 2014.
- United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. Purge and Trap for Aqueous Samples. SW-846 Method 5030C, 2003.
- United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. Closed System Purge and Trap and Extraction for Volatile Organics in Soil and Waste Sample. SW-846 Method 5035A, 2000.
- United States...

14. United States...

14. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Inductively Coupled Plasma-Optical Emission Spectrometry. SW-846 Method 6010D**, 2014.

15. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Flame Atomic Absorption Spectrophotometry. SW-846 Method 7000B**, 2007.

16. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Arsenic (Atomic Absorption, Gaseous Hydride). SW-846 Method 7061A**, 1992.

17. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Chromium, Hexavalent (Colorimetric). SW-846 Method 7196A**, 1992.

18. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Mercury in Liquid Waste (Manual Cold Vapor Technique). SW-846 Method 7470A**, 1994.

19. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Mercury in Solid or Semisolid Waste (Manual Cold-Vapor Technique). SW-846 Method 7471B**, 1998.

20. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Mercury in Solids and Solutions by Thermal Decomposition, Amalgamation, and Atomic Absorption Spectrophotometry. SW-846 Method 7473**, 2007.

21. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Selenium (Atomic Absorption, Borohydride Reduction). SW-846 Method 7742**, 1994.

22. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Nonhalogenated Organics Using GC/FID. SW-846 Method 8015D**, 2003.

23. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Organochlorine Pesticides by Gas Chromatography. SW-846 Method 8081B**, 2007.

24. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Polychlorinated Biphenyls (PCBs) by Gas Chromatography. SW-846 Method 8082A**, 2007.

25. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Organochlorine Pesticides by Gas Chromatography. SW-846 Method 8081B**, 2007.

26. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Chlorinated Herbicides by GC Using Methylation or Pentafluorobenzoylation Derivatization. SW-846 Method 8151A**, 1996. ๑๑๑

27. United States...

27. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Volatile Organic Compounds by Gas Chromatography/ Mass Spectrometry. SW-846 Method 8260D**, 2018.

28. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Semivolatile Organic Compounds by Gas Chromatography/Mass Spectrometry. SW-846 Method 8270E**, 2018.

29. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Cyanide Extraction Procedure for Solids and Oils. SW-846 Method 9013A**, 2014.

30. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Cyanide in Waters and Extracts using Titrimetric and Manual Spectrophotometric Procedures. SW-846 Method 9014**, 2014.

31. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **pH Electrometric Measurement. SW-846 Method 9040C**, 2004.

32. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Soil and Waste pH. SW-846 Method 9045D**, 2004.

๑๑๑

บริษัท อินทิเกรทเต็ด รีเสิร์ช เซ็นเตอร์ จำกัด

ที่ อก ๐๓๑๐(๓)/ ๑๑๐



กรมโรงงานอุตสาหกรรม
ถนนพระรามที่ ๖ แขวงทุ่งพญาไท
เขตราชเทวี กรุงเทพฯ ๑๐๕๐๐

๐๙ มกราคม ๒๕๖๙

เรื่อง ต่ออายุหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน

เรียน กรรมการผู้จัดการ บริษัท อินทิเกรตเต็ด รีเสิร์ช เซ็นเตอร์ จำกัด

อ้างถึง คำขอขึ้นทะเบียน/ต่ออายุ/เปลี่ยนแปลงบุคลากร และชนิดสารมลพิษของห้องปฏิบัติการวิเคราะห์เอกชน
ลงวันที่ ๑๖ ตุลาคม ๒๕๖๘

สิ่งที่ส่งมาด้วย เอกสารแนบท้ายหนังสือต่ออายุรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน
บริษัท อินทิเกรตเต็ด รีเสิร์ช เซ็นเตอร์ จำกัด จำนวน ๓ แผ่น

ตามคำขอที่อ้างถึง บริษัท อินทิเกรตเต็ด รีเสิร์ช เซ็นเตอร์ จำกัด ขอต่ออายุหนังสือ
รับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน เลขทะเบียน ๖-๑๙๙ สถานที่ตั้งเลขที่ ๑๒๒ หมู่ ๒ ตำบลท่าตุม
อำเภอศรีมหาโพธิ จังหวัดปราจีนบุรี ต่อกรมโรงงานอุตสาหกรรม นั้น

กรมโรงงานอุตสาหกรรมพิจารณาแล้ว ให้บริษัท อินทิเกรตเต็ด รีเสิร์ช เซ็นเตอร์ จำกัด ต่ออายุ
หนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน โดยมีองค์ประกอบดังนี้

ก. ผู้ควบคุมห้องปฏิบัติการวิเคราะห์เอกชน

- | | |
|----------------------------------|----------------------------|
| ๑) นางสาววิไลรัตน์ เกียรติอินชัย | ทะเบียนเลขที่ ๖-๑๙๙-๓-๐๐๐๑ |
| ๒) นางสาวติดยา นันหมื่น | ทะเบียนเลขที่ ๖-๑๙๙-๓-๐๐๐๒ |
| ๓) นางวีราภรณ์ ผลเจริญ | ทะเบียนเลขที่ ๖-๑๙๙-๓-๐๐๐๓ |
| ๔) นางสาวชนิกานต์ แสนสุข | ทะเบียนเลขที่ ๖-๑๙๙-๓-๐๐๐๔ |

ข. เจ้าหน้าที่ห้องปฏิบัติการวิเคราะห์เอกชน

- | | |
|---------------------------------|----------------------------|
| ๑) นายไกรวิชญ์ แสงแก้ว | ทะเบียนเลขที่ ๖-๑๙๙-๖-๐๐๐๑ |
| ๒) นางสาวณัฐนันท์ สัจวงษ์ | ทะเบียนเลขที่ ๖-๑๙๙-๖-๐๐๐๒ |
| ๓) นางสาวหนึ่งฤทัย ออบมาลี | ทะเบียนเลขที่ ๖-๑๙๙-๖-๐๐๐๔ |
| ๔) นางสาวแววตา คำสา | ทะเบียนเลขที่ ๖-๑๙๙-๖-๐๐๐๕ |
| ๕) นายจักรีชัย อินดี๊ะ | ทะเบียนเลขที่ ๖-๑๙๙-๖-๐๐๐๖ |
| ๖) นายเจษฎาภรณ์ เปี้ยสุยะ | ทะเบียนเลขที่ ๖-๑๙๙-๖-๐๐๐๘ |
| ๗) นางสาวชลธิชา อนุวัฒน์ธนไพศาล | ทะเบียนเลขที่ ๖-๑๙๙-๖-๐๐๐๙ |
| ๘) นางสาวสุปราณี ทุทธแก่นวงศ์ | ทะเบียนเลขที่ ๖-๑๙๙-๖-๐๐๑๐ |

ค. ขอบข่าย ...



"อุตสาหกรรมก้าวไกล ประเทศไทยก้าวหน้า ร่วมกันพัฒนา อุตสาหกรรมสีเขียว"



- ๒ -

ค. ขอบข่ายชนิดสารมลพิษที่ได้รับขึ้นทะเบียนให้วิเคราะห์ในน้ำเสีย/น้ำทิ้ง
จำนวน ๒๓ รายการ น้ำใต้ดิน จำนวน ๑๓ รายการ สิ่งปฏิภูลหรือวัสดุที่ไม่ใช่แล้ว จำนวน ๙ รายการ
รวมทั้งสิ้น ๔๕ รายการ ตามสิ่งที่ส่งมาด้วย

หนังสือฉบับนี้จะสิ้นสุดอายุในวันที่ ๑๘ พฤศจิกายน ๒๕๗๓ หากประสงค์จะต่ออายุหนังสือ
รับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน ให้ยื่นคำขอต่ออายุพร้อมเอกสารประกอบคำขอต่อกรมโรงงาน
อุตสาหกรรมภายใน ๖๐ วัน ก่อนวันสิ้นสุดอายุของหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน

จึงเรียนมาเพื่อทราบ

ขอแสดงความนับถือ

(นายศิระ จันทร์เฑียร)

นักวิทยาศาสตร์เชี่ยวชาญ วิชาการการแทน
ผู้อำนวยการกองวิจัยและเดือนกัมมลพิษโรงงาน
ปฏิบัติราชการแทนอธิบดีกรมโรงงานอุตสาหกรรม

กองวิจัยและเดือนกัมมลพิษโรงงาน
ศูนย์วิจัยและเดือนกัมมลพิษโรงงานภาคตะวันออก
โทร. ๐ ๓๓๑๓ ๖๐๕๙ ต่อ ๕๐๐๑-๒
ไปรษณีย์อิเล็กทรอนิกส์ eirw@diw.mail.go.th



"อุตสาหกรรมก้าวไกล ประเทศไทยก้าวหน้า ร่วมกันพัฒนา อุตสาหกรรมสีเขียว"



เอกสารแนบท้ายหนังสือต่ออายุรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน
บริษัท อินทีเกรทเต็ด รีเสิร์ช เซ็นเตอร์ จำกัด เลขทะเบียน ว-๑๙๙
ที่ อก ๐๓๑๐(๓)/ ๑๑๐ ลงวันที่ ๐๙ มกราคม ๒๕๖๙

ขอข่ายสารมลพิษที่ได้รับขึ้นทะเบียนจากกรมโรงงานอุตสาหกรรม จำนวน ๔๕ รายการ

น้ำ/น้ำเสีย จำนวน 23 รายการ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
1	Arsenic	Digestion, Inductively Coupled Plasma Method ^[2]
2	Barium	Digestion, Inductively Coupled Plasma Method ^[2]
3	Biochemical Oxygen Demand	1) 5-Day BOD Test, Membrane-Electrode Method ^[2] 2) 5-Day BOD Test, Azide Modification Method ^[2]
4	Cadmium	Digestion, Inductively Coupled Plasma Method ^[2]
5	Chemical Oxygen Demand	Closed Reflux, Colorimetric Method ^[2]
6	Chromium	Digestion, Inductively Coupled Plasma Method ^[2]
7	Color	ADMI Weighted-Ordinate Spectrophotometric Method ^[2]
8	Copper	Digestion, Inductively Coupled Plasma Method ^[2]
9	Free Chlorine	Iodometric Method ^[2]
10	Hexavalent Chromium	Colorimetric Method ^[2]
11	Lead	Digestion, Inductively Coupled Plasma Method ^[2]
12	Manganese	Digestion, Inductively Coupled Plasma Method ^[2]
13	Nickel	Digestion, Inductively Coupled Plasma Method ^[2]
14	Oil and Grease	Liquid-Liquid, Partition-Gravimetric Method ^[2]
15	pH	Electrometric Method ^[2]
16	Selenium	Digestion, Inductively Coupled Plasma Method ^[2]
17	Sulfide	Iodometric Method ^[2]
18	Temperature	Laboratory and Field Methods ^[2]
19	Total Dissolved Solids	Dried at 180 °C ^[2]
20	Total Kjeldahl Nitrogen	Macro-Kjeldahl Method ^[2]
21	Total Suspended Solids	Dried from 103 to 105 °C ^[2]
22	Trivalent Chromium	Calculation ^[2]
23	Zinc	Digestion, Inductively Coupled Plasma Method ^[2]



น้ำใต้ดิน...

- ๒ -

น้ำใต้ดิน จำนวน 13 รายการ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
1	Arsenic	Digestion, Inductively Coupled Plasma Method ^[2]
2	Barium	Digestion, Inductively Coupled Plasma Method ^[2]
3	Cadmium	Digestion, Inductively Coupled Plasma Method ^[2]
4	Chromium	Digestion, Inductively Coupled Plasma Method ^[2]
5	Chromium (III)	Calculation ^[2]
6	Chromium (VI)	Colorimetric Method ^[2]
7	Copper	Digestion, Inductively Coupled Plasma Method ^[2]
8	Lead	Digestion, Inductively Coupled Plasma Method ^[2]
9	Manganese	Digestion, Inductively Coupled Plasma Method ^[2]
10	Nickel	Digestion, Inductively Coupled Plasma Method ^[2]
11	pH	Electrometric Method ^[2]
12	Selenium	Digestion, Inductively Coupled Plasma Method ^[2]
13	Zinc	Digestion, Inductively Coupled Plasma Method ^[2]

สิ่งปฏิกูลหรือวัสดุที่ไม่ใช้แล้ว จำนวน 9 รายการ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
1	Arsenic	1) Digestion, Inductively Coupled Plasma Method ^[3,4] 2) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[1,3,4]
2	Barium	1) Digestion, Inductively Coupled Plasma Method ^[3,4] 2) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[1,3,4]
3	Cadmium	1) Digestion, Inductively Coupled Plasma Method ^[3,4] 2) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[1,3,4]
4	Chromium	1) Digestion, Inductively Coupled Plasma Method ^[3,4] 2) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[1,3,4]
5	Lead	1) Digestion, Inductively Coupled Plasma Method ^[3,4] 2) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[1,3,4]



6 Nikel...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
6	Nickel	1) Digestion, Inductively Coupled Plasma Method ^(3,4) 2) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^(1,3,4)
7	pH	Electrometric Method ⁽⁵⁾
8	Selenium	1) Digestion, Inductively Coupled Plasma Method ^(3,4) 2) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^(1,3,4)
9	Zinc	1) Digestion, Inductively Coupled Plasma Method ^(3,4) 2) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^(1,3,4)

เอกสารอ้างอิง

1. กระทรวงอุตสาหกรรม. ประกาศกระทรวงอุตสาหกรรม, พ.ศ. 2566. เรื่อง การจัดการสิ่งปฏิกูลหรือวัสดุที่ไม่ใช้แล้ว ประกาศในราชกิจจานุเบกษาวันที่ 31 พฤษภาคม 2566. เล่มที่ 140 ตอนพิเศษ 126 ง.
2. APHA, AWWA, WEF. Standard Methods for the Examination of Water and Wastewater. 24th ed. Washington, DC: APHA, 2023.
3. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. Acid Digestion of Sediments, Sludges, and Soils. SW-846 Method 3050B, 1996.
4. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. Inductively Coupled Plasma-Optical Emission Spectrometry. SW-846 Method 6010D, 2018.
5. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. Soil and Waste pH. SW-846 Method 9045D, 2004.