

ภาคผนวกที่ 4

เอกสารสอบเทียบความถูกต้องของเครื่องมือ

**ตารางสรุปรายการเอกสารการสอบเทียบความถูกต้องของเครื่องมือเก็บตัวอย่าง
และเครื่องมือตรวจวิเคราะห์คุณภาพสิ่งแวดล้อม**

รายการตรวจวัด	เครื่องมือเก็บตัวอย่าง	เครื่องมือตรวจวิเคราะห์
	ชื่อเครื่องมือ	ชื่อเครื่องมือ
1. คุณภาพอากาศในบรรยากาศ Total Suspended Particulate	High Volume Air Sampler Blower & Recorder No. B27, R02, R10	Digital Balance
PM ₁₀	PM ₁₀ Air Sampler No. R05, R08, R12	Digital Balance
Carbon Monoxide	Serial No. 171-S, 0926737615, 1201351403	Serial No. 171-S, 0926737615, 1201351403
Sulfur Dioxide	Serial No. 3431, 1310957747, CM06280010	Serial No. 3431, 1310957747, CM06280010
Nitrogen Dioxide	Serial No. 249, 1170530044, CM13090047	Serial No. 249, 1170530044, CM13090047
VOCs	Mass Flow Meter	GC/MS
2. คุณภาพอากาศจากแหล่งกำเนิด Total Suspended Particulate	Console No. R02, R04 Pitot Tube No. B38, B48	Digital Balance
Oxides of Nitrogen	Vacuum Gauge	Spectrophotometer
Sulfur Dioxide	Personal Pump SKC No. R15, R42 Rotameter No. H-R02, R03	-
Carbon Monoxide	Personal Pump SKC No. B78, R28 Rotameter No. H-R02, R03	CO Analyzer No. B02
Lead	Console No. R02, R04 Pitot Tube No. B38, B48	ICP
Mercury	Console No. R02, R04 Pitot Tube No. B38, B48	AAS
3. คุณภาพน้ำ pH	-	pH Meter
Temperature	-	Thermometer
Total Suspended Solids	-	Digital Balance
Total Dissolved Solids	-	Digital Balance
BOD ₅	-	BOD Meter
COD	-	COD Reactor
Grease & Oil	-	Digital Balance
TPH (C ₅ -C ₃₅)	-	GC/MS
4. ระดับเสียงในชุมชน L _{eq} 24 hr, L _{max} และ L ₉₀	Acoustic Calibrator Sound Level Meter No. ACO-R12, R28	-
5. ระดับเสียงเฉลี่ยตลอดระยะเวลาการทำงาน L _{eq} 8 hr	Acoustic Calibrator Sound Level Meter No. ACO-B29, R40	-
TWA	Acoustic Calibrator Sound Level Meter No. ACO-R40, R41	-
6. คุณภาพอากาศในสถานที่ทำงาน Benzene	Personal Pump	GC/FID

คุณภาพอากาศในบรรยากาศ



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

High Volume Air Sampler Calibration Report

Calibration Method : Multipoint Orifice Flow Transfer Standard

Model : TE 5025A

S/N : 3611

Calibration Data

High Volume Air Sampler Data		Calibration Data		
Recorder No.	Blower No.	Date	Actual Flowrate (ft ³ /min)	R ²
B01	B01	03/11/2025	y = 1.118x-3.833	0.997
B02	B02	03/11/2025	y = 1.120x-3.384	0.999
B03	B03	04/11/2025	y = 1.069x-0.968	0.998
B04	B04	03/11/2025	y = 1.096x-2.076	0.996
B05	B05	03/11/2025	y = 1.101x-2.990	0.997
B06	B06	03/11/2025	y = 1.124x-3.707	0.999
B07	B07	03/11/2025	y = 1.133x-2.855	0.999
B08	B08	04/11/2025	y = 1.108x-1.898	0.996
B09	B09	03/11/2025	y = 1.110x-2.993	0.998
B10	B10	03/11/2025	y = 1.116x-3.121	0.999
B11	B11	03/11/2025	y = 1.119x-2.105	0.996
B12	B12	03/11/2025	y = 1.126x-1.525	0.997
B13	B13	05/11/2025	y = 1.093x+0.946	0.998
B14	B14	05/11/2025	y = 1.149x-3.047	0.999
B15	B15	05/11/2025	y = 1.137x-3.875	0.999
B16	B16	03/11/2025	y = 1.079x-2.409	0.998
B17	B17	03/11/2025	y = 1.177x-4.168	0.997
B18	B18	03/11/2025	y = 1.138x-2.900	0.999
B19	B19	03/11/2025	y = 1.109x-1.623	0.996
B20	B20	03/11/2025	y = 1.123x-0.045	0.999
B21	B21	04/11/2025	y = 1.082x+0.484	0.998
B22	B22	04/11/2025	y = 1.110x-1.594	0.996
B23	B23	04/11/2025	y = 1.135x-2.878	0.999
B24	B24	04/11/2025	y = 1.141x-3.242	0.998
B25	B25	03/11/2025	Y = 1.011x+3.037	0.997
B26	B26	03/11/2025	y = 1.104x-2.679	0.998
B27	B27	03/11/2025	y = 1.148x-3.947	0.999
B28	B28	03/11/2025	y = 1.120x-3.393	0.998
B29	B29	05/11/2025	y = 1.142x-3.319	0.997
B30	B30	05/11/2025	y = 1.139x-1.015	0.996
B31	B31	05/11/2025	y = 1.152x-2.962	0.997
B32	B32	05/11/2025	y = 1.140x-3.712	0.999
B33	B33	05/11/2025	y = 1.125x-0.806	0.996
B34	B34	04/11/2025	y = 1.150x-3.245	0.996

Calibrated by :

Adul Dangklom
(Mr. Adul Dangklom)

Approved by :

Peera Detudom
(Mr. Peera Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด

S.P.S. CONSULTING SERVICE CO., LTD.

7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900

7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900

Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

High Volume Air Sampler Calibration Report

Calibration Method : Multipoint Orifice Flow Transfer Standard

Model : TE 5025A

S/N : 3611

Calibration Data

High Volume Air Sampler Data		Calibration Data		
Recorder No.	Blower No.	Date	Actual Flowrate (ft ³ /min)	R ²
B35	B35	04/11/2025	$y = 1.088x - 1.183$	0.997
B36	B36	04/11/2025	$y = 1.131x - 2.774$	0.996
B37	B37	04/11/2025	$y = 1.068x + 0.301$	0.999
B38	B38	03/11/2025	$y = 1.109x - 3.757$	0.998
B39	B39	03/11/2025	$y = 1.027x + 0.098$	0.999
B40	B40	04/11/2025	$y = 1.117x - 1.067$	0.997
B41	B41	04/11/2025	$y = 1.097x - 1.570$	0.997
B42	B42	04/11/2025	$y = 1.142x - 3.608$	0.997
B43	B43	05/11/2025	$y = 1.100x - 0.506$	0.998
B44	B44	05/11/2025	$y = 1.149x - 3.077$	0.999
R01	R01	05/11/2025	$y = 1.114x - 0.751$	0.998
R02	R02	03/11/2025	$y = 1.144x - 3.923$	0.999
R03	R03	03/11/2025	$y = 1.161x - 4.126$	0.999
R04	R04	03/11/2025	$y = 1.113x - 2.188$	0.997
R05	R05	03/11/2025	$y = 1.139x - 0.779$	0.999
R06	R06	03/11/2025	$y = 1.106x - 1.148$	0.996
R07	R07	03/11/2025	$y = 1.128x - 3.641$	0.999
R08	R08	03/11/2025	$y = 1.135x - 4.572$	0.996
R09	R09	03/11/2025	$y = 1.121x - 4.112$	0.998
R10	R10	03/11/2025	$y = 1.117x - 2.052$	0.999
R11	R11	03/11/2025	$y = 1.110x - 2.812$	0.996
R12	R12	03/11/2025	$y = 1.120x - 1.259$	0.996
R13	R13	04/11/2025	$y = 1.146x - 5.407$	0.998
R14	R14	04/11/2025	$y = 1.150x - 3.484$	0.999
R15	R15	04/11/2025	$y = 1.143x - 5.066$	0.998
R16	R16	04/11/2025	$y = 1.153x - 6.481$	0.996
R17	R17	03/11/2025	$y = 1.126x - 3.877$	0.998
R18	R18	03/11/2025	$y = 1.147x - 5.065$	0.997
R19	R19	03/11/2025	$y = 1.119x - 4.625$	0.999
R20	R20	03/11/2025	$y = 1.148x - 4.605$	0.997

Calibrated by :

Adul Dangklom
(Mr. Adul Dangklom)

Approved by :

Peera Detudom
(Mr. Peera Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด

S.P.S. CONSULTING SERVICE CO., LTD.

7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900

7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900

Tel : (662) 939-4370-72. Fax : (662) 513-4221. E-mail : sale@spscon.com. www.spscon.com

High Volume PM-10 Air Sampler Calibration Report

Calibration Method : Multipoint Orifice Flow Transfer Standard

Model : TE 5025A

S/N : 3611

Calibration Data

High Volume PM-10 Data		Calibration Data		
Recorder No.	Blower No.	Date	Actual Flowrate (ft ³ /min)	R ²
R01	R01	03/11/2025	$y = 1.055x + 0.899$	0.998
R02	R02	03/11/2025	$y = 1.132x - 3.919$	0.998
R03	R03	03/11/2025	$y = 1.113x - 2.991$	0.996
R04	R04	03/11/2025	$y = 1.126x - 3.936$	0.996
R05	R05	04/11/2025	$y = 1.103x - 2.678$	0.996
R06	R06	04/11/2025	$y = 1.107x - 1.644$	0.996
R07	R07	04/11/2025	$y = 1.085x - 0.497$	0.998
R08	R08	03/11/2025	$y = 1.071x + 0.571$	0.998
R09	R09	03/11/2025	$y = 1.116x - 2.909$	0.999
R10	R10	03/11/2025	$y = 1.089x - 1.636$	0.996
R11	R11	03/11/2025	$y = 1.045x + 1.442$	0.999
R12	R12	03/11/2025	$y = 1.058x - 0.370$	0.998
R13	R13	03/11/2025	$y = 1.100x - 2.187$	0.998
R14	R14	03/11/2025	$y = 1.099x - 1.650$	0.999
R15	R15	03/11/2025	$y = 1.128x - 4.768$	0.997
R16	R16	05/11/2025	$y = 1.093x - 2.124$	0.997
R17	R17	05/11/2025	$y = 1.101x - 2.286$	0.997
R18	R18	05/11/2025	$y = 1.118x - 5.339$	0.999
R19	R19	03/11/2025	$y = 1.054x + 1.212$	0.996
R20	R20	03/11/2025	$y = 1.068x - 1.764$	0.997

Calibrated by :

Adul Dangklom
(Mr. Adul Dangklom)

Approved by :


Peera Detudom
(Mr. Peera Detudom)




บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72. Fax : (662) 513-4221. E-mail : sale@spscon.com. www.spscon.com

Calibration Report					
Non-Dispersive Infrared CO Analyzer					
Date :	30 November 2025	Brand :	API	Model :	300E
No.	CO-R02			Serial No.	171-S
Calibrator (Dilution System)					
Brand : Teledyne			Model : 700E		
Last Cal. Date : 29 October 2025			Serial No. : 201-S		
Reference Standard Gas					
Standard Gas : Carbon Monoxide (CO)			Cylinder No. : D711839		
Certified Date : 14 March 2024		Expired Date : 14 March 2032		Cylinder Conc. : 4,580 ppm	
Calibrating Condition					
Pressure	1011	mmbar	Temp.	24.6	°C
			% RH	50	
Calibration Setting					
Span	Initial Reading (Before Adj.), PPM			Final Reading (After Adj.), PPM	
Set Point	Expected Concentration	Analyzer Response	%Dif	Analyzer Response	
Zero	0	-0.10	-	0	
CO Span	40.00	40.05	0.125	40.00	
API Model 300E CO Analyzer Check List					
Parameter	Observed Value	Units	Nominal Range		
Range	50	PPM	0-1000 ppm		
Stability	0.10	PPM	< 1 ppm With Zero Air		
CO Measure	4016.2	mV	2500-4800 mV		
CO Reference	3948.8	mV	2500-4800 mV		
Measure/Reference Ratio	1.180	-	1.1-1.3 W/Zero Air		
Sample Pressure	28.5	In-Hg-A	~2" < Ambient Absolute Pressure		
Sample Flow	808	CC/Min	800 ± 10%		
Sample Temperature	48.4	°C	48 ± 4		
Bench Temperature	48.2	°C	48 ± 2		
Wheel Temperature	68.3	°C	68 ± 2		
Box Temperature	30.8	°C	Ambient Temp + 7 ± 10		
Photo-Drive	3045.7	mV	250 mV to 4750 mV		
Slope	1.017	-	1.0 ± 0.3		
Offset	0.2	-	0 ± 0.3		

Calibrated by :


(Mr.Kaseam Simaphon)

Approved by :


(Mr.Yuthana Thanataranit)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

CALIBRATION REPORT					
SO ₂ FLUORESCENT ANALYZER					
DATE :	30 November 2025	BRAND :	API	MODEL :	100E
NO.	SO ₂ -R02			SERIAL NO.	3431
Calibrator (Dilution System)					
Brand	: Teledyne			Model	: 700E
Last Cal. Date	: 29 October 2025			Serial No.	: 201-S
Reference Standard Gas					
Standard Gas	: Sulphur Dioxide (SO ₂)			Cylinder No.	: A00814SK
Certified Date	: 21 June 2021	Expired Date	: 21 June 2029	Cylinder Conc.	: 49.8 ppm
CALIBRATING CONDITION					
Pressure	1011	mmbar	Temp.	24.6	°C
			% RH	50	
CALIBRATION SETTING					
Span	Initial Reading (Before Adj.),PPB			Final Reading (After Adj.),PPB	
Set Point	Expected Concentration	Analyzer Response	%Dif	Analyzer Response	Slope
Zero	0	-0.10	-	0	-
SO ₂ Span	400.0	400.1	0.025	400.0	1.005
API Model 100E SO ₂ Analyzer Check list					
Test Values	Observed Value	Units	Nominal Range		
RANGE	500	PPB	0-500		
SAMPLE PRESS	28.6	in-Hg	25-35		
SAMPLE FLOW	654	cc/min	650 ± 10%		
PMT	103.3	mV	-20-150 with Zero Air		
UV LAMP	2892.3	mV	1000-4900		
STR. LGT	60.9	PPB	<100		
DRK PMT	62.7	mV	-50 - 200		
DRK LMP	57.6	mV	-50 - 200		
HVPS	672	V	550-900 constant		
DCPS	2517	mV	2500 ± 200		
RCCELL TEMP	50.0	°C	50 ± 1		
BOX TEMP	29.2	°C	5-40		
PMT TEMP	7.2	°C	7 ± 2.0		
SO ₂ Span Conc	400	PPB	20-20,000		
SO ₂ Slope	1.005	-	1.0 ± 0.3		
SO ₂ Offset	21.8	mV	<250		
Stability at Zero	0.1	PPB	<0.2		
Stability at Span	0.2	PPB	0.5% of reading (above 50 ppb)		

Calibrated by :

(Mr.Kaseam Simaphon)

Approved by :

(Mr.Yuthana Thanataranit)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

CALIBRATION REPORT					
CHEMILUMINESCENT NO / NO ₂ / NO _x ANALYZER					
DATE :	30 November 2025	BRAND :	API	MODEL :	200E
NO.	NOX-B16	SERIAL NO.	249		
Calibrator (Dilution System)					
Brand	: Teledyne			Model	: 700E
Last Cal. Date	: 29 October 2025			Serial No.	: 201-S
Reference Standard Gas					
Standard Gas	: Nitric Oxide (NO)			Cylinder No.	: A00674SV
Certified Date	: 12 March 2025	Expired Date	: 12 March 2028	Cylinder Conc.	: 48.7 ppm
CALIBRATING CONDITION					
Pressure	1011	mmbar	Temp.	24.6	°C
% RH	50				
CALIBRATION SETTING					
Span	Initial Reading (Before Adj.),PPB			Final Reading (After Adj.),PPB	
Set Point	Expected Concentration	Analyzer Response	%Dif	Analyzer Response	Slope
Zero	0	0.11	-	0	-
NO Span	400	399.9	-0.025	400.0	1.005
NO _x Span	400	400.2	0.050	400.0	1.009
API Model 200E NO _x Analyzer Check List					
Test Values	Observed Value	Units	Nominal Range		
RANGE	500	PPB	500 standard		
STABILITY (Zero Gas)	0.1	PPB	< 2 with zero air		
SAMPLE FLOW	505	cc/min	500 ± 50		
OZONE FLOW	79	cc/min	80 ± 15		
PMT	103.5	mV	-20 - 150		
AZERO	94.0	mV	-20 - 150		
HVPS	671	V	420 - 900 constant		
RCELL TEMP	50.3	°C	50 ± 1		
BOX TEMP	28.6	°C	8 - 48		
PMT TEMP	7.4	°C	7 ± 2		
MOLY TEMP	315.2	°C	315 ± 5		
RCELL PRESS	8.6	IN-Hg-A	2 - 10 constant		
SAMPLE PRESS	28.4	IN-Hg-A	25 - 30 constant		
NO Span Conc	400	PPB	20 - 20,000		
NO _x Span Conc	400	PPB	20 - 20,000		
NO Slope	1.005	-	1.0 ± 0.3		
NO _x Slope	1.009	-	1.0 ± 0.3		
NO Offset	1.0	mV	-20 to +150		
NO _x Offset	0.6	mV	-20 to 150		
Stability at Zero	0.1	PPB	< 0.2		
Stability at Span	0.2	PPB	< 2 ppb @ 400 ppb span gas		

Calibrated by :

(Mr.Kaseam Simaphon)

Approved by :

(Mr.Yuthana Thanataranit)



CERTIFICATE No : 25M2254

REFERENCE No : 76365-1

PAGE : 1 OF 2

Certificate of Calibration

EQUIPMENT : DIGITAL BALANCE

MANUFACTURER : METTLER TOLEDO

MODEL : XS105DU

SERIAL No : 1126422905


ID No : BA05/50

CONDITION AS RECEIVED : USED ITEM

SUBMITTED BY : S.P.S. CONSULTING SERVICE CO., LTD.
7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN RD.,
JOMPOL, CHATUCHAK, BANGKOK 10900

CALIBRATED BY : ATSAWIN Y.

CALIBRATION DATE : 07-Mar-25

APPROVED BY : 
PONGSAK J.

ISSUED DATE : 13-Mar-25

RECEIVED DATE : 07-Mar-25

THIS CERTIFICATE MAY NOT BE REPRODUCED OTHER THAN IN FULL EXCEPT WITH THE PRIOR WRITTEN APPROVAL OF
QUALITY CALIBRATION CO., LTD.





CERTIFICATE No : 25M2254

PAGE : 2 OF 2

Calibration Report

EQUIPMENT : DIGITAL BALANCE MODEL : XS105DU
MANUFACTURER : METTLER TOLEDO S/N : 1126422905
ID No : BA05/50 RECEIVED DATE : 07-Mar-25
AIR PRESSURE : 1009mbar $\pm$ 1mbar CALIBRATION DATE : 07-Mar-25
AMBIENT TEMPERATURE : 24° C $\pm$ 1° C RELATIVE HUMIDITY : 54 %RH $\pm$ 10 % RH

CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED BY ACCORDING TO UKAS LAB 14 EDITION 6:2019 BY USING KNOWN WEIGHT STANDARD WEIGHT. THE BALANCE WAS NOT ADJUSTED BEFORE CALIBRATION. THE BALANCE HAS NO ZERO TRACKING FUNCTION. REPEATABILITY WAS MEASURED BY USING 10 REPEATED MEASUREMENTS. LINEARITY WAS MEASURED COVERING 10 POINTS, EVENLY SPREAD OVER THE RANGE. THE INSTRUMENT WAS SET ZERO BEFORE PERFORMING THE LINEARITY TEST. OFF-CENTER LOADING WAS MEASURED BY USING STANDARD WEIGHTS PLACED ON THE PAN AND MOVED TO VARIOUS POSITIONS ON THE PAN.

2. REFERENCE STANDARD INSTRUMENTS :-

<u>INSTRUMENT</u>	<u>MODEL</u>	<u>SERIAL No</u>	<u>CERTIFICATE No</u>	<u>DUE DATE</u>
1) STANDARD WEIGHT SET	E2	QK-I-151	C02250116	28-Jan-27
2) STANDARD WEIGHT	E2	15843	C02250117	29-Jan-27

3. THE CERTIFICATE IS VALID FOR THE ITEM CALIBRATED AS SHOWN ON THE DATE AND PLACE OF CALIBRATION ONLY.

4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.

5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-

- NATIONAL INSTITUTE OF METROLOGY (THAILAND)

RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

1. ZERO SETTING FUNCTION : NORMAL


2. TARE FUNCTION : NORMAL

3. REPEATABILITY OF READING AT 120 g WAS 0.000055 g

4. DEPARTURE FROM NOMINAL VALUE/ LINEARITY

NOMINAL VALUE (g)	BALANCE READING (g)	CORRECTION (g)	UNCERTAINTY ($\pm$ g)
0.00	0.00000	0.00000	0.000065
0.02	0.01999	0.00001	0.000065
0.10	0.10001	-0.00001	0.000066
0.20	0.20001	-0.00001	0.000066
0.50	0.50002	-0.00002	0.000065
1.00	1.00003	-0.00003	0.000066
2.00	2.00001	-0.00001	0.000067
5.00	5.00002	-0.00002	0.000068
10.00	10.00000	0.00000	0.000070
20.00	20.00004	-0.00004	0.000078
50.00	50.00000	0.00000	0.00013
100.00	100.0001	-0.0001	0.00019
120.00	120.0002	-0.0002	0.00022

5. OFF CENTER LOADING ERROR




POINT	READING (g)
1	50.0000
2	50.0000
3	50.0000
4	50.0000
5	50.0000
OFF-CENTER LOADING	0.0000

NOTE: THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA
THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR $k=2$, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT





MIRACLE INTERNATIONAL TECHNOLOGY CO.,LTD

214 Bangwaek Rd. Bangpai Bangkae Bangkok 10160
Tel.: 0-2865-4647-8 Fax: 0-2865-4649 <http://www.mit.in.th>



CALIBRATION CERTIFICATE

Page 1 of 4

Certificate No. : L202412119-0001

Date Issued : 13-Dec-24

Customer : S.P.S. CONSULTING SERVICE CO., LTD.
7 Soi Phaholyothin 24 Phaholyothin Road., Jompol, Chatuchak,
Bangkok 10900

Equipment : Mass Flow meter

Manufacturer : Dwyer

Model : GMF-2101

Serial No. : -

ID No./Tag No. : MF01/51

Date Received : 11-Dec-24

Date Calibrated : 12-Dec-24

Calibrated by : Saruth Srichutikul

Calibration Method or Calibration Procedure Used

In-house method : CP-34 by comparison against mass flow calibrator.

This certificate is traceable to national standards, which realize the units of measurement according to the International System of Units (SI).

Result of Calibration

The reported uncertainty of measurement was based on standard uncertainty multiplied by a coverage factor $k = 2$, providing a level confidence approximately 95 percent.

This certificate may not be reproduced other than in full except with the prior written approval of the Miracle International Technology Company Limited.

Approved by:

Sarayuth T.
(Sarayuth Tochua)



Certificate No. : L202412119-0001

Ambient Temperature : $(25 \pm 2)^{\circ}\text{C}$

Relative Humidity : $(50 \pm 15)\%\text{RH}$

Capacity Range : 17 ml/min

Calibration Media : Air


Type : Mass Flowmeter

Unit Under Calibration Reference Condition : Pressure 101.325 kPa(abs) , 21°C , Nitrogen

Before Adjustment

Temperature ($^{\circ}\text{C}$)	Pressure (kPa)	UUC Reading (ml/min)	STD Reading (ml/min)	Error (ml/min)	Uncertainty ($\pm$ ml/min)
24.00	100.46	0.00	0.000 *	0.000	0.063
24.10	100.62	3.30	3.149	0.151	0.13
24.10	100.78	7.30	7.2	0.10	0.14
24.20	101.07	13.50	13.7	-0.20	0.15
24.20	101.30	17.00	18.3	-1.30	0.19

Error = Unit Under Calibration - Standard

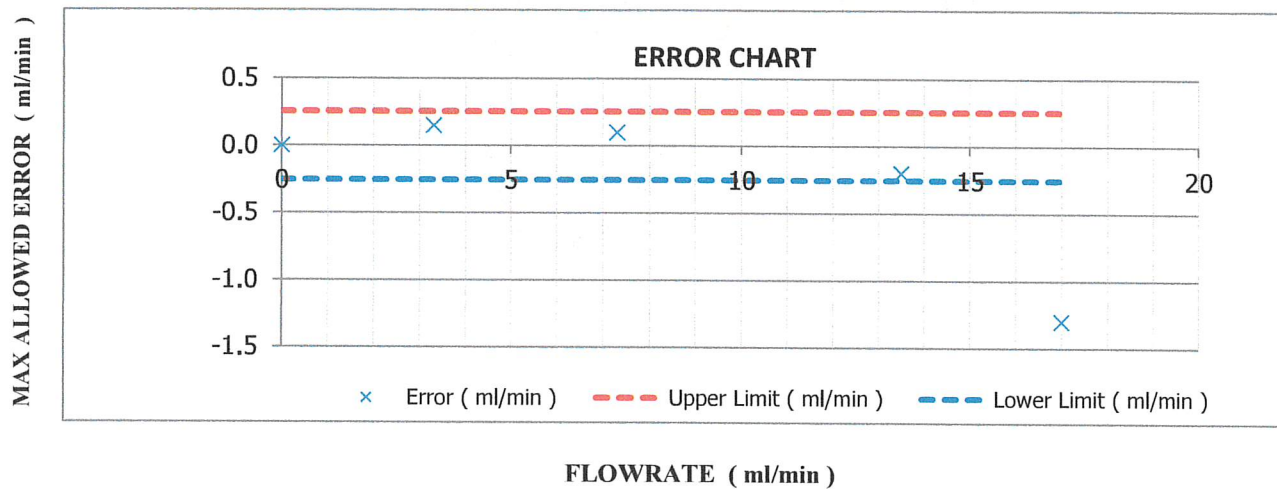

Certificate No. : L202412119-0001

Ambient Temperature : (25 ± 2)°C

Relative Humidity : (50 ± 15)%RH

Capacity Range : 17 ml/min

Calibration Media : Air


Type : Mass Flowmeter

Unit Under Calibration Reference Condition : Pressure 101.325 kPa(abs) , 21 °C , Nitrogen

After Adjustment

Temperature (° C)	Pressure (kPa)	UUC Reading (ml/min)	STD Reading (ml/min)	Error (ml/min)	Uncertainty (± ml/min)
24.00	100.45	0.00	0.000 *	0.000	0.063
24.10	100.62	3.30	3.170	0.130	0.13
24.10	100.78	7.30	7.2	0.10	0.14
24.20	101.01	13.50	13.6	-0.10	0.15
24.00	101.19	17.00	17.1	-0.10	0.18

Error = Unit Under Calibration - Standard

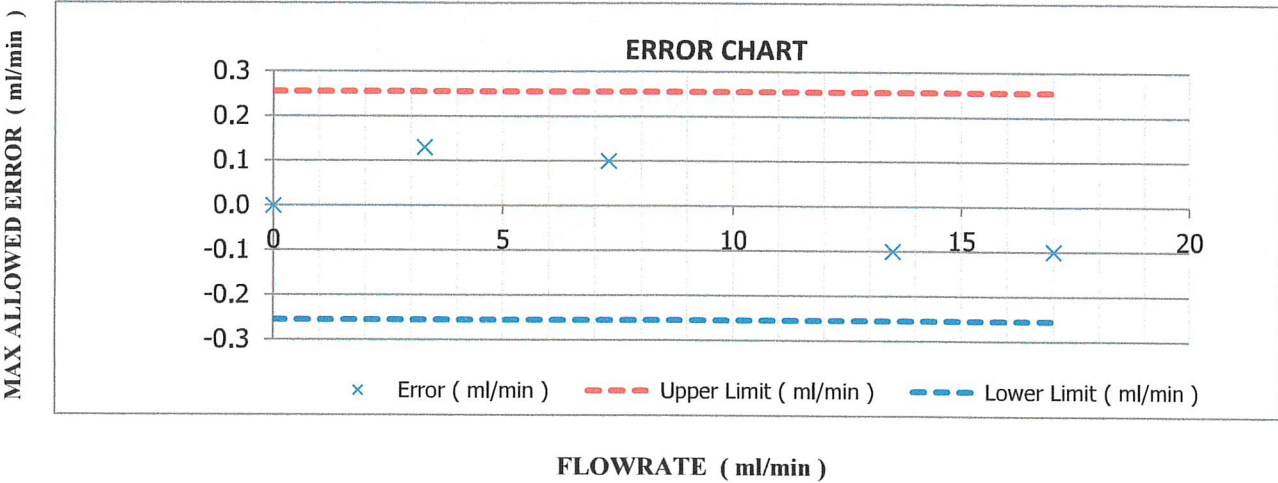

Certificate No. : L202412119-0001

Note : The actual flow rate is determined by the equation :

$$Q_{Meas} = Q_{Ref} \times \frac{P_{Ref}}{P_{Meas}} \times \frac{T_{Meas}}{T_{Ref}}$$

; Q = Flow rate

; P = Absolute pressure

; T = Absolute temperature

; Subscript "Meas" = Measurement condition

; Subscript "Ref" = Reference condition

Condition As-Received : Used Item


The measurement results and statements of conformity with specification only relate to the item calibrated.

Traceability of Certificate :

The International System of Units (SI) through

NIMT Certificate No. MW-0047-24, MW-0048-24 for Gas Flow meter Serial No. M5209179B/M5209179A, Due 03-Jul-25

End of Certificate



MIRACLE INTERNATIONAL TECHNOLOGY CO.,LTD

214 Bangwaek Rd. Bangpai Bangkae Bangkok 10160
Tel.: 0-2865-4647-8 Fax: 0-2865-4649 <http://www.mit.in.th>



CALIBRATION CERTIFICATE

Page 1 of 3

Certificate No. : L202511307-0001

Date Issued : 01-Dec-25

Customer : S.P.S. CONSULTING SERVICE CO., LTD.
7 Soi Phaholyothin 24 Phaholyothin Road., Jompol, Chatuchak, Bangkok
10900

Equipment : Mass Flow meter

Manufacturer : Dwyer

Model : GMF-2101

Serial No. : -

ID No./Tag No. : MF01/51

Date Received : 27-Nov-25

Date Calibrated : 30-Nov-25

Calibrated by : Nattawat Laochai

Calibration Method or Calibration Procedure Used

In-house method : CP-34 by comparison against mass flow calibrator.

This certificate is traceable to national standards, which realize the units of measurement according to the International System of Units (SI).

Result of Calibration

The reported uncertainty of measurement was based on standard uncertainty multiplied by a coverage factor $k = 2$, providing a level confidence approximately 95 percent.

This certificate may not be reproduced other than in full except with the prior written approval of the Miracle International Technology Company Limited.

Approved by:

K. Nathong
(Nathapong Krudaum)



Certificate No. : L202511307-0001

Ambient Temperature : $(25 \pm 2)^{\circ}\text{C}$

Relative Humidity : $(50 \pm 15)\%\text{RH}$

Capacity Range : 17 ml/min

Calibration Media : Nitrogen


Type : Mass Flowmeter

Unit Under Calibration Reference Condition : Pressure 101.325 kPa(abs) , 21 °C , Nitrogen

Temperature (° C)	Pressure (kPa)	UUC Reading (ml/min)	STD Reading (ml/min)	Error (ml/min)	Uncertainty (± ml/min)
24.69	101.22	0.00	0.000 *	0.000	0.063
24.44	119.03	3.30	3.358	-0.058	0.14
24.38	118.17	7.30	7.4	-0.10	0.15
24.30	156.08	13.50	13.6	-0.10	0.15
24.25	169.92	17.00	17.1	-0.10	0.18

Error = Unit Under Calibration - Standard

Marked * are not included in the NSC-ONSC accreditation schedule for our laboratory.

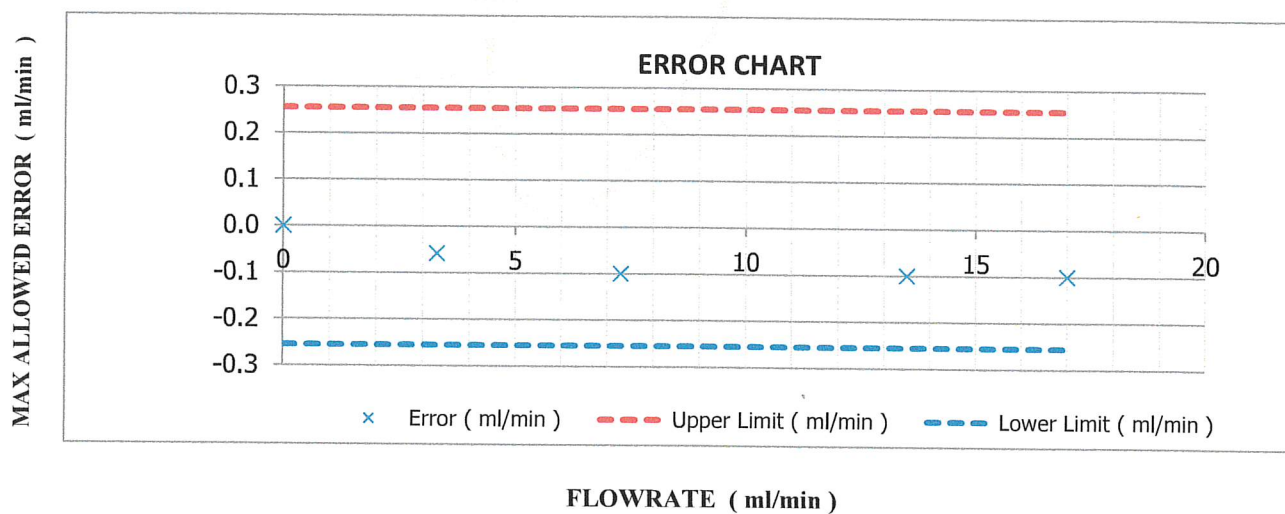

Certificate No. : L202511307-0001

Note : The actual flow rate is determined by the equation :

$$Q_{Meas} = Q_{Ref} \times \frac{P_{Ref}}{P_{Meas}} \times \frac{T_{Meas}}{T_{Ref}}$$

; Q = Flow rate

; P = Absolute pressure

; T = Absolute temperature

; Subscript "Meas" = Measurement condition

; Subscript "Ref" = Reference condition

Condition As-Received : Used Item

The measurement results and statements of conformity with specification only relate to the item calibrated.

Traceability of Certificate :

The International System of Units (SI) through

NIMT Calibration Certificate No. MW-0047-24 for Gas Flow meter Serial No. M5209179B/M5209179A, Due 28-Jun-26

NIMT Calibration Certificate No. MW-0048-24 for Gas Flow meter Serial No. M5209179C/M5209179A, Due 02-Jul-26

End of Certificate

GC Clarus 600/680 Preventive Maintenance (PM)

Company Name:	S.P.S. Consulting Service Co.,Ltd		
Address (Instrument Location):	7 Soi Phaholyothin24 Phaholyothin Road, Jompol, Chatuchak, Bangkok, 10900.		
Serial Number:	680S14042502	Service Tag:	N68APSSFEMP
Customer Name (if applicable):	Ms.Naruecha	PM number:	1 of 2
Service Engineer Name:	Monchai Kitcharoenkeat	Service Order Number:	WO-
Date PM Performed: (DD-MMM-YYYY)	22-Feb-2025	Next PM Due Date: (DD-MMM-YYYY)	22-Aug-2025

Part Number	Release	Publication Date	
TH09370070	C	August 2016	

Scope

The purpose of this PM is to ensure the continued functionality of the Clarus 600 and Clarus 680 GC by inspecting and replacing any worn or damaged parts. This service should only be performed by a trained representative of PerkinElmer. The customer should save their method before the PM begins.

General Instructions:

The customer must provide the engineer operational data to demonstrate recent instrument performance prior to starting the PM. Always check with the customer before making any changes that may affect the customer's analysis or calibration, including a current back-up of system software and/or data files. The completed document should be signed by an authorized PerkinElmer and customer representative and left with the customer. Update the PM sticker and instrument logbook as required.

Copyright Information

This document contains proprietary information that is protected by copyright. All rights are reserved. No part of this publication may be reproduced in any form whatsoever or translated into any language without the prior, written permission of Perkin Elmer, Inc. **Copyright © 2013 PerkinElmer, Inc.**

Trademarks

Registered names, trademarks, etc. used in this document, even when not specifically marked as such, are protected by law. PerkinElmer is a registered trademark of PerkinElmer, Inc. All other trademarks and registered trademarks not owned by PerkinElmer, Inc. or its subsidiaries that are depicted herein are the property of their respective owners. **Except as specifically set forth in its terms and conditions of sale, PerkinElmer makes no Warranty of any kind with regard to this document, including, but not limited to, the implied warranties of merchantability and fitness for a particular purpose.** PerkinElmer shall not be liable for incidental or consequential damages in connection with the furnishing or use of this document.

Component List

Component / Specific Model	Serial #	Software Version	Configuration Notes
Clarus680	680S14042502	Totalchrom6.3.2	PSS, PSS, FID,
Clarus SQ8T	648N4050804	Turbomass 6.4	
AtomX	US14113002	Tekma AtomX	

Parts Lists

Additional Tools Required for PM				
Part Number (if applicable)	Description	Quantity	Serial #	Calibration Due Date (MM/YY)
N/A				
Additional Reagents and Standards Required for PM				
Part Number (if applicable)	Description	Quantity	Batch/Lot #	Expiration Date (MM/YY)
N/A				

Procedure Checklist

Use (✓) to check off those steps in the checklist that have been completed.

1. General:

- ☒ Review the instrument performance with the customer and document any recent problems.

- ☒ Check incoming AC line voltage for proper levels and grounding.

L-N 220 Volt

L-G 220 Volt

N-G 0.33 Volt

**Neutral to ground not more than 0.5 volts peak to peak*

- ☒ Inspect all gas line filters and traps; Replace if necessary with customer supplied spares.

Carrier gas ☒ Helium ☐ Nitrogen ☐ Hydrogen

Moisture level ☒ Good ☐ Need to replace ☐ Other _____

Detector gas ☒ Air Zero ☒ Hydrogen ☐ Nitrogen ☐ Helium

Moisture level ☒ Good ☐ Need to replace ☐ Other _____

- ☒ Inspect the customer log book and make any appropriate PM entries.

- ☒ Leak check all fittings from the gas source to instrument.

Gas leakage ☒ Pass ☐ Fail Comment _____

- ☒ Perform general inspection of system for cleanliness.

- ☒ Inspect for functional and clean electronic cooling and oven vent fans

Electronic cooling fan ☒ Yes ☐ No

Oven cooling fan ☒ Yes ☐ No

2. Electronic :

- ☒ Check oven temperature. Calibrate if necessary.

Oven temperature set point 150 °C ☒ Pass ☐ Fail

- ☐ Check sub-ambient option. (If installed).

Oven temperature set point 5 °C ☐ Pass ☐ Fail

- ☒ Perform routine maintenance on detector/injector. Replace parts as necessary with customer supplied spares.

- ☒ Check flows, including split flows if applicable. Calibrate if necessary.

Carrier flow	Pass
Split flow	Pass
- ☒ Check detector gas flows and adjust if necessary.

Detector flow	Pass
---------------	------
- ☒ Autosampler installed ☒ Yes ☐ No

Check autosampler sensor for wear and replace if necessary.	
Vial sensor	Pass
Door sensor	Pass
Tower sensor	Pass
Plunger sensor	Pass
Elevator sensor	Pass
- ☒ Remove syringe, manually flush. Replace with customer supplied spare if necessary.
- ☒ Check firmware version. Upgrade to current levels if necessary.

Firmware version	<u>6.5</u>
------------------	------------
- ☒ Measure all accessible power supply voltages.

5 Volt	Pass
+15 Volt	Pass
-15 Volt	Pass
24 Volt	Pass
- ☒ Record all detector voltage signal.

Detector Channel A	<u>1.12</u>	mV.
Detector Channel B	<u>NA</u>	mV.

3. Diagnostics Tests:

- ☒ Run instrument diagnostics.

☒ BRAM	Pass
☒ EPROM	Pass
- ☒ Run Autosampler diagnostics.

☒ BRAM	Pass
☒ EPROM	Pass

4. Review:

- ☒ Review with the customer PM work performed.
- ☒ Review with the customer routine maintenance procedures.
- ☒ Discuss recommended customer-supplied materials to have on hand
- ☒ Attach PM sticker.
- ☒ Update Logbook.

Additional Comments

Additional Comments Regarding the PM

Review

<i>The preventive maintenance checks and if applicable performance tests for Clarus600/680 GC have been completed.</i>		
<i>This Clarus600/680 GC Pass the preventive maintenance.</i>		
Review of Preventive Maintenance:		
Authorized PerkinElmer Representative: Monchai Kitcharoenkeat	<i>Monchai</i>	Date: 22-Feb-2025 (DD-MMM-YYYY)
Authorized Customer Representative: Ms.Naruecha	<i>Naruecha</i>	Date: 22-Feb-2025 (DD-MMM-YYYY)

GC Clarus 600/680 Preventive Maintenance (PM)

Company Name:	S.P.S. Consulting Service Co.,Ltd		
Address (Instrument Location):	7 Soi Phaholyothin24 Phaholyothin Road, Jompol, Chatuchak, Bangkok, 10900.		
Serial Number:	680S14042502	Service Tag:	N68APSSFEMP
Customer Name (if applicable):	Ms.Naruecha	PM number:	2 of 2
Service Engineer Name:	Monchai Kitcharoenkeat	Service Order Number:	WO-06815714
Date PM Performed: (DD-MMM-YYYY)	13-Aug-2025	Next PM Due Date: (DD-MMM-YYYY)	13-Feb-2026

Part Number	Release	Publication Date	
TH09370070	C	August 2016	

Scope

The purpose of this PM is to ensure the continued functionality of the Clarus 600 and Clarus 680 GC by inspecting and replacing any worn or damaged parts. This service should only be performed by a trained representative of PerkinElmer. The customer should save their method before the PM begins.

General Instructions:

The customer must provide the engineer operational data to demonstrate recent instrument performance prior to starting the PM. Always check with the customer before making any changes that may affect the customer's analysis or calibration, including a current back-up of system software and/or data files. The completed document should be signed by an authorized PerkinElmer and customer representative and left with the customer. Update the PM sticker and instrument logbook as required.

Copyright Information

This document contains proprietary information that is protected by copyright. All rights are reserved. No part of this publication may be reproduced in any form whatsoever or translated into any language without the prior, written permission of Perkin Elmer, Inc. **Copyright © 2013 PerkinElmer, Inc.**

Trademarks

Registered names, trademarks, etc. used in this document, even when not specifically marked as such, are protected by law. PerkinElmer is a registered trademark of PerkinElmer, Inc. All other trademarks and registered trademarks not owned by PerkinElmer, Inc. or its subsidiaries that are depicted herein are the property of their respective owners. **Except as specifically set forth in its terms and conditions of sale, PerkinElmer makes no Warranty of any kind with regard to this document, including, but not limited to, the implied warranties of merchantability and fitness for a particular purpose.** PerkinElmer shall not be liable for incidental or consequential damages in connection with the furnishing or use of this document.

Component List

Component / Specific Model	Serial #	Software Version	Configuration Notes
Clarus680	680S14042502	Totalchrom6.3.2	PSS, PSS, FID,
Clarus SQ8T	648N4050804	Turbomass 6.4	
AtomX	US14113002	Tekma AtomX	

Parts Lists

Additional Tools Required for PM				
Part Number (if applicable)	Description	Quantity	Serial #	Calibration Due Date (MM/YY)
N/A				
Additional Reagents and Standards Required for PM				
Part Number (if applicable)	Description	Quantity	Batch/Lot #	Expiration Date (MM/YY)
N/A				

Procedure Checklist

Use (✓) to check off those steps in the checklist that have been completed.

1. General:

- ☒ Review the instrument performance with the customer and document any recent problems.

- ☒ Check incoming AC line voltage for proper levels and grounding.

L-N 220 Volt

L-G 220 Volt

N-G 0.32 Volt

**Neutral to ground not more than 0.5 volts peak to peak*

- ☒ Inspect all gas line filters and traps; Replace if necessary with customer supplied spares.

Carrier gas ☒ Helium ☐ Nitrogen ☐ Hydrogen

Moisture level ☒ Good ☐ Need to replace ☐ Other _____

Detector gas ☒ Air Zero ☒ Hydrogen ☐ Nitrogen ☐ Helium

Moisture level ☒ Good ☐ Need to replace ☐ Other _____

- ☒ Inspect the customer log book and make any appropriate PM entries.

- ☒ Leak check all fittings from the gas source to instrument.

Gas leakage ☒ Pass ☐ Fail Comment _____

- ☒ Perform general inspection of system for cleanliness.

- ☒ Inspect for functional and clean electronic cooling and oven vent fans

Electronic cooling fan ☒ Yes ☐ No

Oven cooling fan ☒ Yes ☐ No

2. Electronic :

- ☒ Check oven temperature. Calibrate if necessary.

Oven temperature set point 150 °C ☒ Pass ☐ Fail

- ☐ Check sub-ambient option. (If installed).

Oven temperature set point 5 °C ☐ Pass ☐ Fail

- ☒ Perform routine maintenance on detector/injector. Replace parts as necessary with customer supplied spares.

- ☒ Check flows, including split flows if applicable. Calibrate if necessary.

Carrier flow	Pass
Split flow	Pass
- ☒ Check detector gas flows and adjust if necessary.

Detector flow	Pass
---------------	------
- ☒ Autosampler installed ☒ Yes ☐ No

Check autosampler sensor for wear and replace if necessary.	
Vial sensor	Pass
Door sensor	Pass
Tower sensor	Pass
Plunger sensor	Pass
Elevator sensor	Pass
- ☒ Remove syringe, manually flush. Replace with customer supplied spare if necessary.
- ☒ Check firmware version. Upgrade to current levels if necessary.

Firmware version	<u>6.5</u>
------------------	------------
- ☒ Measure all accessible power supply voltages.

5 Volt	Pass
+15 Volt	Pass
-15 Volt	Pass
24 Volt	Pass
- ☒ Record all detector voltage signal.

Detector Channel A	<u>0.98</u>	mV.
Detector Channel B	<u>NA</u>	mV.

3. Diagnostics Tests:

- ☒ Run instrument diagnostics.

☒ BRAM	Pass
☒ EPROM	Pass
- ☒ Run Autosampler diagnostics.

☒ BRAM	Pass
☒ EPROM	Pass

4. Review:

- ☒ Review with the customer PM work performed.
- ☒ Review with the customer routine maintenance procedures.
- ☒ Discuss recommended customer-supplied materials to have on hand
- ☒ Attach PM sticker.
- ☒ Update Logbook.

Additional Comments

Additional Comments Regarding the PM

Review

<i>The preventive maintenance checks and if applicable performance tests for Clarus600/680 GC have been completed.</i>	
<i>This Clarus600/680 GC Pass the preventive maintenance.</i>	
<i>Review of Preventive Maintenance:</i>	
Authorized PerkinElmer Representative: Monchai Kitcharoenkeat <i>Monchai</i>	Date: 13-Aug-2025 (DD-MMM-YYYY)
Authorized Customer Representative: Ms.Naruecha <i>Naruecha</i>	Date: 13-Aug-2025 (DD-MMM-YYYY)



บริษัท คิว-ชี โซลูชั่นส์ จำกัด

Q-SHE SOLUTIONS CO., LTD.

7/409 ซอยวิภาวดีรังสิต 36 ถนนวิภาวดีรังสิต แขวงจตุจักร เขตจตุจักร กรุงเทพฯ 10900

โทรศัพท์ : (662) 939-5711 (12 Lines) โทรสาร : (662) 939-4207-8


Website <http://www.qshe.co.th> E-mail-address: info@qshe.co.th

รายงานการสอบเทียบก๊าซแบบหลายจุด
MULTI-POINT GAS TEST REPORT

Date :	11 August 2025	Temperature(°C) :	26	Pressure(mBar) :	-
Equipment :	Gas Analyzer (CO	Model S/N :	48i, 0926737615		
Manufacturer :	Thermc	Location :	Micro		

Standard Gas Concentration			Dilutor Details	
Sulfur Dioxide (SO ₂)	44.44	ppm.	Manufacture	Thermc
Nitric Oxide (NO	45.84	ppm.	Model	146i
Carbon Monoxide (CO	4513	ppm.	Serial Number	1201351404
Methane (CH ₄)	506.7	ppm.	Zero Air	
Cylinder NO	CC507818		Manufacture	Thermc
Expiration Date	August 13, 2025		Model / Serial Number	111-B2R

Multi Point Gas Test Data									Result Test Report		
Reference Value (ppb.)			Analyzer Displa			Difference Error (ppm.	Percent Error	Percent Abs.(STD≤15%)			
			#1	#2	AVG.						
Level 1	Zero	0	0.09	-	0.09	0.09	-	-	Percent	Percent	Percent
Level 2	20%	10	9.80	-	9.80	-0.20	-2.00	2.00	Corre.	Slope	Inter.
Level 3	40%	20	19.70	-	19.70	-0.30	-1.50	1.50	Error	Error	Error
Level 4	60%	30	29.80	-	29.80	-0.20	-0.67	0.67	STD	STD	STD
Level 5	80%	40	40.02	-	40.02	0.02	0.05	0.05	<+0.5%	<+5%	<+3%
Average Difference (%)								1.05	-0.0054	-0.1400	-2.2222
Intercept		-0.0900			Slope		0.9986	Correlation Coefficient		0.9999	

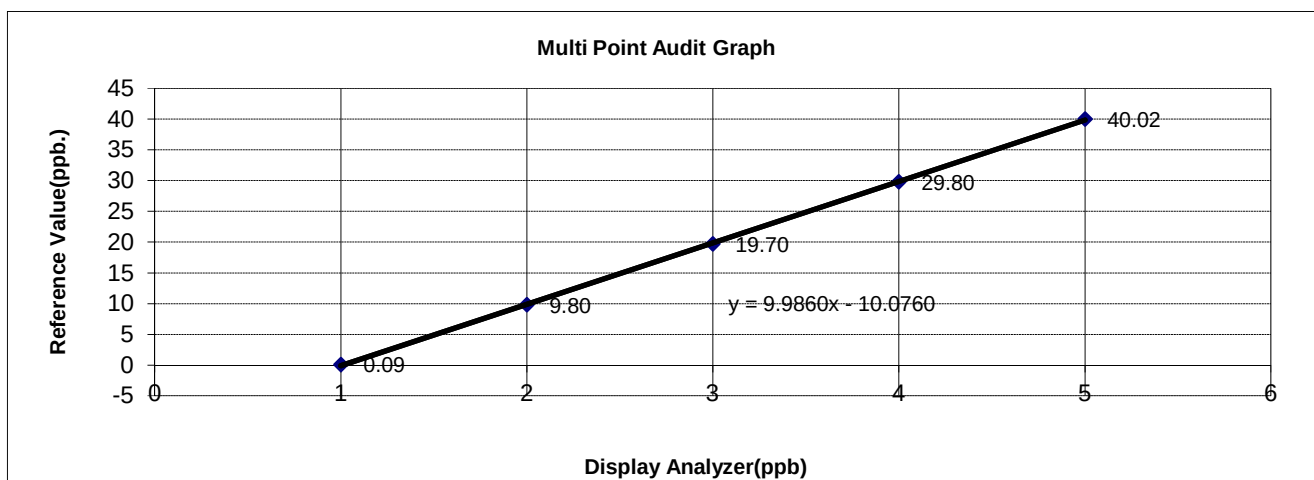

Calibrate by : ชินธร มุขโรจน์
Date : 11 August 2025

Job Number :	J092500024-003	Customer Name :	IRPC
Equipment :	AQMs Station.	Contact Name :	KhunWirasakKhumsuk
Model :	AQMs Station.	Telephone Number :	081-803-0475
Serial Number :	Pluak Kate Station	E-mail address/Fax. :	wirasak.k@irpc.co.th
Working Date :	03 December 2025	Working Hour :	4 Hours

Service Report

Working Scope:

Service Station

Physical Checking:

- ตรวจเช็ค Data logger พบว่าทำงานได้ปกติ
- ตรวจเช็ค Diagnostic of all analyzers อยู่ในเกณฑ์ปกติ
- ตรวจเช็ค Reading of all analyzers และ Met sensor พบว่าปกติ
- ตรวจเช็ค ผล Calibration พบว่าอยู่ในเกณฑ์ปกติ
- ตรวจเช็ค Dilutor และ Zero Air พบว่าทำงานได้ปกติ
- ตรวจเช็ค เครื่องวัดฝุ่น PM-10 พบว่าทำงานได้ปกติ
- ตรวจเช็ค เครื่อง THC analyzer พบว่าทำงานได้ปกติ
- ตรวจเช็ค การทำงานของระบบไฟฟ้า และ UPS พบว่าทำงานได้ปกติ
- ทำความสะอาดภายในสถานี และ บริเวณรอบสถานี

Correction working:

Calibrate single-point of all analyzers.	Drain water for pump of Zero Air.
Replace sample filter 47 mm.	Clean หัววัดฝุ่น
Replace diaphragm pump of CO.	

Part Replacements:

- Sample Filter 47 mm. 6 ea. (Part support by IRPC)
- Diaphragm pump of CO. 1 ea. (Part support by IRPC)

Addition Recommended:

- End -

Serviced by :	ชินโรส มุขโรจน์	Serviced Date	03 December 2025
Approved by:		Approved Date :	03 December 2025



บริษัท คิว-ซี โซลูชั่นส์ จำกัด

7/409 ซอยวิภาวดีรังสิต 36 ถนนวิภาวดีรังสิต แขวงจตุจักร เขตจตุจักร กรุงเทพฯ 10900

โทรศัพท์ : (662) 939-5711 (12 Lines) โทรสาร : (662) 939-4207-8

Website <http://www.qshe.co.th> E-mail-address: info@qshe.co.th

General Checking

Equipment :	AQMs Pluak Kate	Model :	-
Serial Number :	Pluak Kate Station	Manufacturer :	-

Item	Description	Set-Point Value	Status & Value	Remark
	<u>On Mobile</u>			
1	Air conditioner operation	OK	OK	
2	Mobile temperature	25-27 °C	26°C	
3	Lighting system	OK	OK	
4	Lamp in sampling box	OK	OK	
5	Sampling probe	Clean	Clean	
6	Blower	OK	OK	
7	Drain liquid in tank	Drain	Drain	
8	Compressor tank set pressure	80 psi	Fail	
9	Zero air compressor operation	OK	OK	นำของบ้านแลงมาใช้แทนชั่วคราว
10	Silica gel for dry air of NO _x analyzer	OK	OK	
11	UPS 3 KVA	OK	OK	
12	Data logger	OK	OK	
13	Ventilation fan	OK	OK	
14	Power cable	OK	OK	
15	Hydrogen Gas	-	350/40 psi	
16	Standard gas#1 (NO,SO ₂ ,HC,CO)	-	1900/32 psi	

Note :

NO-NO₂-NO_x Analyzer

Equipment :	NO-NO ₂ -NO _x analyzer.	Model :	42i
Serial Number :	1170530044	Manufacturer :	Thermo Scientific

Diagnostic test value				
Parameter	Observed value		Unit	Nominal range
	Before	After		
Sample reading				
NO reading	12.1	15.1	ppb	
NO _x reading	23.7	44.3	ppb	
Range	500	500	ppb	50 to 1000 ppb
Averaging Time	30	30	Sec	10 to 300 Sec
Calibration Factors				
NO BKG. ppb	19.7	18.6	ppb	0 to 60
NO _x BKG. ppb	23.8	19.3	ppb	0 to 60
NO COEF.	1.217	1.172	-	1.0 ± 0.3
NO _x COEF.	0.975	0.915	-	1.0 ± 0.3
NO ₂ COEF.	1.000	1.000	-	1.0 ± 0.3
Instrument Controls				
Ozonator	On	On		On/Off
PMT Supply	On	On		On/Off
Auto/Manual Mode	NO/NO _x	NO/NO _x		NO/NO _x , NO, NO _x
Baud Rate	9600	9600	bps	1200 to 9600
Temp Compensation	On	On	-	On/Off
Pressure Compensation	On	On	-	On/Off
Screen Contrast	45	45	%	0 to 100
Service Mode	Off	Off	-	On/Off, Up to used
Diagnostics				
Voltages				
PMT Supply	-903.2	-903.2	Vdc	-400 to -1200 Vdc
5 Supply	4.9	4.9	Vdc	5.0 ± 1 Vdc
15 Supply	15.1	15.1	Vdc	15.0 ± 1 Vdc
-15 Supply	-15.0	-15.0	Vdc	-15.0 ± 1 Vdc
Temperatures				
Internal	34.5	35.2	°C	15 °C to 45 °C
Chamber	49.9	49.8	°C	50°C ± 2 °C
Cooler	-2.9	-2.8	°C	(-)3 °C ± 2 °C
Converter	327.4	323.2	°C	325 °C ± 5 °C
Converter Set	325.0	325.0	°C	325 °C
Pressure	272.0	272.8	mmHg	250 ± 100 mmHg
Flow	0.558	0.565	L/min	0.5 to 1.00 L/min

Note :



บริษัท คิว-ชี โซลูชั่นส์ จำกัด

7/409 ซอยวิภาวดีรังสิต 36 ถนนวิภาวดีรังสิต แขวงจตุจักร เขตจตุจักร กรุงเทพฯ 10900

โทรศัพท์ : (662) 939-5711 (12 Lines) โทรสาร : (662) 939-4207-8

Website <http://www.qshe.co.th> E-mail-address: info@qshe.co.th

SO₂ Analyzer

Equipment : Sulfur Dioxide analyzer.

Model : 43I-BZSAB

Serial Number : CM06280010

Manufacturer : Thermo Scientific

Diagnostic test value				
Parameter	Observed value		Unit	Nominal range
	Before	After		
Sample reading	4.9	2.4	ppb	
Range	500	500	ppb	50 to 1000 ppb
Averaging Time	30	30	Sec	10 to 300 Sec
Calibration Factors				
SO ₂ BKG. ppb	25.4	26.2	ppb	0 to 60
SO ₂ COEF	1.011	1.039	-	1.0 ± 0.3
Instrument Controls				
Temp Correction	On	On	On/Off	On
Pressure Correction	On	On	On/Off	On
Flash Lamp	On	On	On/Off	On
Communication setting				
Baud Rate	9600	9600	bps	9600 to 115000
Instrument ID	43	43	-	0 to 99
Screen Brightness	50	50	%	0 to 100
Service Mode	Off	Off	On/Off	Up to used
Diagnostics				
Voltages				
Motherboard voltages:				
3.3 Supply	3.3	3.3	Vdc	3.3 +/- 1 Vdc
5.0 Supply	5.0	5.0	Vdc	5.0 +/- 1 Vdc
15.0 Supply	15.1	15.1	Vdc	15.0 +/- 1 Vdc
24.0 Supply	23.9	23.9	Vdc	24.0 +/- 1 Vdc
-3.3 Supply	-3.2	-3.2	Vdc	- 3.3 +/- 1 Vdc
Interface board voltages:				
PMT Supply	-602.0	-602.0		
Flash Supply	823	821		
3.3 Supply	3.3	3.3	Vdc	3.3 +/- 1 Vdc
5.0 Supply	5.0	5.0	Vdc	5.0 +/- 1 Vdc
15.0 Supply	14.7	14.7	Vdc	15.0 +/- 1 Vdc
-15.0 Supply	-15.0	-15.0	Vdc	-15.0 +/- 1 Vdc
24.0 Supply	23.9	23.9	Vdc	24.0 +/- 1 Vdc
Temperatures				
Internal	36.8	37.8	°C	15°C to 45°C
Chamber	45.3	45.2	°C	45°C ± 2°C
Pressure	731.3	733.1	mmHg	750 ± 100 mmHg
Flow	0.624	0.624	L/min	0.5 to 1.00 L/min
Lamp intensity	91	91	%	40 – 100 %

Note :



บริษัท คิว-ชี โซลูชั่นส์ จำกัด

7/409 ซอยวิภาวดีรังสิต 36 ถนนวิภาวดีรังสิต แขวงจตุจักร เขตจตุจักร กรุงเทพฯ 10900

โทรศัพท์ : (662) 939-5711 (12 Lines) โทรสาร : (662) 939-4207-8

Website <http://www.qshe.co.th> E-mail-address: info@qshe.co.th

CO Analyzer

Equipment :	CO analyzer.	Model :	48i
Serial Number :	1201351403	Manufacturer :	Thermo Scientific

Diagnostic test value				
Parameter	Observed value		Unit	Nominal range
	Before	After		
Sample reading	0.711	0.478	ppm	
Range	50.0	50.0	ppm	0 to 100 ppm
Averaging Time	60	60	Sec	10 to 300 Sec
Calibration Factors				
CO BKG. ppm	1.656	1.773	ppm	0 to 60
CO COEF	1.013	1.016	-	1.0 ± 0.3
Instrument Controls				
Temp Compensation	On	On	-	On/Off
Pressure Compensation	On	On	-	On/Off
Baud Rate	9600	9600	bps	1200 to 115200 bps
Instrument ID	48	48	-	0 to 99
Screen Contrast	40	40	%	0 to 100 %
Service Mode	Off	Off	-	On/Off, Up to used
Diagnostics				
Voltages				
Motherboard voltages:				
3.3 Supply	3.3	3.3	Vdc	3.3 +/- 1 Vdc
5.0 Supply	5.0	5.0	Vdc	5.0 +/- 1 Vdc
15.0 Supply	14.9	14.9	Vdc	15.0 +/- 1 Vdc
24.0 Supply	24.1	24.1	Vdc	24.0 +/- 1 Vdc
-3.3 Supply	-3.2	-3.2	Vdc	- 3.3 +/- 1 Vdc
Interface board voltages:				
3.3 Supply	3.3	3.3	Vdc	3.3 +/- 1 Vd
5.0 Supply	4.9	4.9	Vdc	5.0 +/- 1 Vdc
15.0 Supply	15.0	15.0	Vdc	15.0 +/- 1 Vdc
24.0 Supply	24.1	24.1	Vdc	24.0 +/- 1 Vdc
-15.0 Supply	-15.1	-15.1	Vdc	-15.0 ± 1.0 Vdc
18.0 IR Supply	18.1	18.1	Vdc	18.0 ± 1.0 Vdc
18.0 MOT Supply	21.7	20.5	Vdc	18.0 ± 5.0 Vdc
Bias Supply	-107.5	-107.5	Vdc	-100 to -110 Vdc
Temperatures				
Internal	38.9	39.4	°C	
Bench	48.5	48.6	°C	
Pressure	761.5	747.9	mmHg	760 ± 100 mmHg.
Flow	0.080	0.826	L/min	1 ± 0.3 L/min
S/R Ratio	1.1294100	1.1297300	-	1.140 – 1.180
AGC intensity	199799	199756	Hz	200,000 ±50,000 Hz
Motor speed	100.01	100.01	%	100 ± 5%

Note :



บริษัท คิว-ซี โซลูชั่นส์ จำกัด

7/409 ซอยวิภาวดีรังสิต 36 ถนนวิภาวดีรังสิต แขวงจตุจักร เขตจตุจักร กรุงเทพฯ 10900

โทรศัพท์ : (662) 939-5711 (12 Lines) โทรสาร : (662) 939-4207-8

Website <http://www.qshe.co.th> E-mail-address: info@qshe.co.th

SINGLE-POINT GAS CALIBRATION

All analyzer.

Equipment :	All analyzer.	Model :	42C, 43i , 48i, 49i
Serial Number :	0504710413,CM06280010, 1201351403,CM09040067	Manufacturer :	Thermo

Standard gas concentration			Dilutor detail	
Sulfur Dioxide (SO ₂)	44.7	ppm	Manufacturer :	Thermo
Nitric Oxide (NO)	45.0	ppm	Model :	146C
Methane (CH ₄)	498	ppm	Serial number :	0504710414
Carbon oxide (CO)	4550	ppm		
Cylinder NO. :	A00931SK			
Expiration Date :	8 Sep 2026			

BEFORE CALIBRATION RESULT

PARAMETER	ZERO			SPAN			JUDGEMENT
	IDEAL	ACTUAL	ERROR	IDEAL	ACTUAL	%ERROR	
NO (ppb)	0.00			400			
NO _x (ppb)	0.00			400			
SO ₂ (ppb)	0.00			400			
CO (ppm)	0.00			40.3			
O ₃ (ppb)	0.00			400			
CH ₄ (ppm)	0.00			5.00			
THC (ppm)	0.00			5.00			

AFTER CALIBRATION RESULT

PARAMETER	ZERO			SPAN			JUDGEMENT
	IDEAL	ACTUAL	ERROR	IDEAL	ACTUAL	%ERROR	
NO (ppb)	0.00	0.9	0.90	400	399.0	-0.25	Valid
NO _x (ppb)	0.00	1.7	1.70	400	402.0	0.50	Valid
SO ₂ (ppb)	0.00	1.2	1.20	400	401.0	0.25	Valid
CO (ppm)	0.00	0.20	0.20	40.3	40.4	0.25	Valid
O ₃ (ppb)	0.00	1.0	1.00	400	399.0	-0.25	Valid
CH ₄ (ppm)	0.00			5.00			
THC (ppm)	0.00			5.00			

Remark :



บริษัท คิว-ชี โซลูชั่นส์ จำกัด

7/409 ซอยวิภาวดีรังสิต 36 ถนนวิภาวดีรังสิต แขวงจตุจักร เขตจตุจักร กรุงเทพฯ 10900

โทรศัพท์ : (662) 939-5711 (12 Lines) โทรสาร : (662) 939-4207-8

Website <http://www.qshe.co.th> E-mail-address: info@qshe.co.th

Job Number :	J092500024-003	Customer Name :	IRPC
Equipment :	Micro Mobile AQMs	Contact Name :	Khun Wirasak Khumsuk
Model :	Micro Mobile AQMs	Telephone Number :	081-803-0475
Serial Number :	Micro Mobile3	E-mail address/Fax. :	wirasak.k@irpc.co.th
Working Date :	11 December 2025	Working Hour :	4 Hours

Service Report

Working Scope:

รถเคลื่อนที่ AQMs micro#3 จอดตรวจวัดอากาศ อยู่ที่ อนามัยหนองจอก จึงได้เข้าทำการตรวจเช็ค

Physical Checking:

- ตรวจเช็ค Data logger พบว่าทำงานได้ปกติ
- ตรวจเช็ค Diagnostic of all analyzers อยู่ในเกณฑ์ปกติ
- ตรวจเช็ค Reading of all analyzers และ Met sensor พบว่าปกติ
- ตรวจเช็ค เครื่องวัดฝุ่น PM-10 พบว่าทำงานได้ปกติ
- ตรวจเช็ค เครื่อง THC analyzer พบว่าทำงานได้ปกติ
- ตรวจเช็ค การทำงานของระบบไฟฟ้า และ UPS พบว่าทำงานได้ปกติ
- ทำความสะอาดภายในสถานี และ บริเวณรอบสถานี

Correction working:

Replace silica gel for dryer NO _x Analyzer.	Drain water for pump of Zero Air.
Replace sample filter 47 mm.	

Part Replacement:

- | | | |
|-------------------------|-------------|------------------------|
| - Sample filter 47 mm. | 3 ea. | (Part Support by IRPC) |
| - Silica gel. P/N: 6998 | 1/2 Bottle. | (Part Support by IRPC) |

Addition Recommended:

-- End --

Serviced by :	ชินโรส มุขโรจน์	Serviced Date :	11 December 2025
Approved by:		Approved Date :	11 December 2025



บริษัท คิว-ซี โซลูชันส์ จำกัด

7/409 ซอยวิภาวดีรังสิต 36 ถนนวิภาวดีรังสิต แขวงจตุจักร เขตจตุจักร กรุงเทพฯ 10900

โทรศัพท์ : (662) 939-5711 (12 Lines) โทรสาร : (662) 939-4207-8

Website <http://www.qshe.co.th> E-mail-address: info@qshe.co.th

General Checking

Equipment : Micro Mobile AQMS

Model : -

Serial Number : -

Manufacturer : -

Item	Description	Set-Point Value	Status & Value	Remark
	<u>On Mobile</u>			
1	Air conditioner operation	OK	OK	
2	Mobile temperature	25-27 °C	25-27 °C	
3	Lighting system	OK	OK	
4	Lamp in sampling box	OK	OK	
5	Sampling probe	Clean	Clean	
6	Blower	OK	OK	
7	Drain liquid in tank	Drain	Drain	
8	Compressor tank set pressure	80 psi	80 psi	
9	Zero air compressor operation	OK	OK	
10	Silica gel for dry air of NO _x analyzer	OK	OK	
11	UPS 6 KVA	Bypass	Bypass	
12	Data logger	OK	OK	
13	Ventilation fan	OK	OK	
14	Power cable	OK	OK	
15	Hydrogen Gas	>500 psi	500/50 psi	
16	Standard gas#1 (NO,SO ₂ ,HC,CO)	>500 psi	300/22 psi	

Note :



บริษัท คิว-ชี โซลูชั่นส์ จำกัด

7/409 ซอยวิภาวดีรังสิต 36 ถนนวิภาวดีรังสิต แขวงจตุจักร เขตจตุจักร กรุงเทพฯ 10900

โทรศัพท์ : (662) 939-5711 (12 Lines) โทรสาร : (662) 939-4207-8

Website <http://www.qshe.co.th> E-mail-address: info@qshe.co.th

NO-NO₂-NO_x AnalyzerEquipment : NO-NO₂-NO_x analyzer.

Model : 42i

Serial Number : CM13090047

Manufacturer : Thermo

Diagnostic test value

Parameter	Observed value		Unit	Nominal range
	Before	After		
Sample reading				
NO reading	7.5	5.8	ppb	
NO _x reading	9.5	7.9	ppb	
Range	500	500	ppb	50 to 1000 ppb
Averaging Time	60	60	Sec	10 to 300 Sec
Calibration Factors				
NO BKG. ppb	49.8	49.8	ppb	0 to 60
NO _x BKG. ppb	44.8	44.8	ppb	0 to 60
NO COEF.	0.948	0.948	-	1.0 ± 0.3
NO _x COEF.	1.000	1.000	-	1.0 ± 0.3
NO ₂ COEF.	1.000	1.000	-	1.0 ± 0.3
Instrument Controls				
Ozonator	On	On		On/Off
PMT Supply	On	On		On/Off
Auto/Manual Mode	NO/NO _x	NO/NO _x		NO/NO _x , NO, NO _x
Baud Rate	9600	9600	bps	1200 to 9600
Temp Compensation	On	On	-	On/Off
Pressure Compensation	On	On	-	On/Off
Screen Contrast	55	55	%	0 to 100
Service Mode	Off	Off	-	On/Off, Up to used
Diagnostics				
Voltages				
Motherboard voltages:				
3.3 Supply	3.3	3.3	Vdc	3.3 ± 1 Vdc
5.0 Supply	5.0	5.0	Vdc	5.0 ± 1 Vdc
15.0 Supply	14.9	14.9	Vdc	15.0 ± 1 Vdc
24.0 Supply	24.1	24.1	Vdc	24.0 ± 1 Vdc
-3.3 Supply	-3.2	-3.2	Vdc	-3.3 ± 1 Vdc
Interface board voltages:				
PMT Supply	-906.5	-906.5	Vdc	-400 to -1200 Vdc
3.3 Supply	3.3	3.3	Vdc	3.3 ± 1 Vdc
5.0 Supply	5.0	5.0	Vdc	5.0 ± 1 Vdc
15.0 Supply	14.9	14.9	Vdc	15.0 ± 1 Vdc
P15.0 Supply	15.2	15.2	Vdc	15.0 ± 1 Vdc
24.0 Supply	23.3	23.3	Vdc	24.0 ± 1 Vdc
-15.0 Supply	-15.2	-15.2	Vdc	-15.0 ± 1 Vdc
Temperatures				
Internal	27.8	28.0	°C	15 °C to 45 °C
Chamber	49.6	49.7	°C	50°C ± 2 °C
Cooler	-2.7	-2.7	°C	(-)3 °C ± 2 °C
Converter	323.4	325.1	°C	325 °C ± 5 °C
Converter Set	325.0	325.0	°C	325 °C
Pressure	315.8	318.8	mmHg	250 ± 100 mmHg
Flow	0.548	0.548	L/min	0.5 to 1.00 L/min

Note :



บริษัท คิว-ชี โซลูชันส์ จำกัด

7/409 ซอยวิภาวดีรังสิต 36 ถนนวิภาวดีรังสิต แขวงจตุจักร เขตจตุจักร กรุงเทพฯ 10900

โทรศัพท์ : (662) 939-5711 (12 Lines) โทรสาร : (662) 939-4207-8

Website <http://www.qshe.co.th> E-mail-address: info@qshe.co.th

SO₂ Analyzer

Equipment : Sulfur Dioxide analyzer.

Model : 43i

Serial Number : 1310957747

Manufacturer : Thermo

Diagnostic test value				
Parameter	Observed value		Unit	Nominal range
	Before	After		
Sample reading	7.6	7.1	ppb	
Range	500	500	ppb	50 to 1000 ppb
Averaging Time	30	30	Sec	10 to 300 Sec
Calibration Factors				
SO ₂ BKG. ppb	110.0	109.7	ppb	0 to 60
SO ₂ COEF	0.977	0.977	-	1.0 ± 0.3
Instrument Controls				
Temp Compensation	On	On	On/Off	On
Pressure Compensation	On	On	On/Off	On
Flash Lamp	On	On	On/Off	On
Communication setting				
Baud Rate	9600	9600	bps	9600 to 115000
Instrument ID	43	43	-	0 to 99
Screen Contrast	50	50	%	0 to 100
Service Mode	Off	Off	On/Off	Up to used
Diagnostics				
Voltages				
Motherboard voltages:				
3.3 Supply	3.3	3.3	Vdc	3.3 +/- 1 Vdc
5.0 Supply	5.0	5.0	Vdc	5.0 +/- 1 Vdc
15.0 Supply	15.1	15.1	Vdc	15.0 +/- 1 Vdc
24.0 Supply	23.7	23.7	Vdc	24.0 +/- 1 Vdc
-3.3 Supply	-3.1	-3.1	Vdc	- 3.3 +/- 1 Vdc
Interface board voltages:				
PMT Supply	-685.2	-685.2		
Flash Supply	842	845		
3.3 Supply	3.2	3.2	Vdc	3.3 +/- 1 Vd
5.0 Supply	5.0	5.0	Vdc	5.0 +/- 1 Vdc
15.0 Supply	14.7	14.7	Vdc	15.0 +/- 1 Vdc
-15.0 Supply	-15.0	-15.0	Vdc	-15.0 +/- 1 Vdc
24.0 Supply	23.2	23.2	Vdc	24.0 +/- 1 Vdc
Temperatures				
Internal	31.8	32.0	°C	15°C to 45°C
Chamber	44.9	45.0	°C	45°C ± 2°C
Pressure	0.0	0.0	mmHg	750 ± 100 mmHg
Flow	0.513	0.513	L/min	0.5 to 1.00 L/min
Lamp intensity	88	89	%	40 – 100 %

Note : หน้าจอมืด มองไม่ชัดเจน



บริษัท คิว-ชี โซลูชันส์ จำกัด

7/409 ซอยวิภาวดีรังสิต 36 ถนนวิภาวดีรังสิต แขวงจตุจักร เขตจตุจักร กรุงเทพฯ 10900

โทรศัพท์ : (662) 939-5711 (12 Lines) โทรสาร : (662) 939-4207-8

Website <http://www.qshe.co.th> E-mail-address: info@qshe.co.th

SINGLE-POINT GAS CALIBRATION

NO_x, SO₂, CO Analyzer.

Equipment :	All analyzer.	Model :	42i, 43i,THC
Serial Number :	--	Manufacturer :	Thermo, Horiba

Standard gas concentration			Dilutor detail	
Sulfur Dioxide (SO ₂)	44.44	ppm	Manufacturer :	Thermo
Nitric Oxide (NO)	45.84	ppm	Model :	146i
Methane (CH ₄)	506.7	ppm	Serial number :	1201351404
Carbon Monoxide (CO)	4513	ppm		
Cylinder NO. :	CC507818			
Expiration Date :	13 Aug 2023			

BEFORE CALIBRATION RESULT

PARAMETER	ZERO			SPAN			JUDGEMENT
	IDEAL	ACTUAL	ERROR	IDEAL	ACTUAL	%ERROR	
NO (ppb)	0.00			400			
NO _x (ppb)	0.00			400			
SO ₂ (ppb)	0.00			400			
CH ₄ (ppm)	0.00			4.43			
THC(ppm)	0.00			4.43			

AFTER CALIBRATION RESULT

PARAMETER	ZERO			SPAN			JUDGEMENT
	IDEAL	ACTUAL	ERROR	IDEAL	ACTUAL	%ERROR	
NO (ppb)	0.00			400			
NO _x (ppb)	0.00			400			
SO ₂ (ppb)	0.00			400			
CH ₄ (ppm)	0.00			4.00			
THC(ppm)	0.00			4.00			

Remark:



บริษัท คิว-ชี โซลูชั่นส์ จำกัด

7/409 ซอยวิภาวดีรังสิต 36 ถนนวิภาวดีรังสิต แขวงจตุจักร เขตจตุจักร กรุงเทพฯ 10900

โทรศัพท์ : (662) 939-5711 (12 Lines) โทรสาร : (662) 939-4207-8

Website <http://www.qshe.co.th> E-mail-address: info@qshe.co.th

คุณภาพอากาศจากแหล่งกำเนิด



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด

S.P.S. CONSULTING SERVICE CO., LTD.

7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900

7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900

Tel : (662) 939-4370-72. Fax : (662) 513-4221, E-mail : sale@spscon.com., www.spscon.com

Console Calibration Report

Calibration Method

Critical Orifices

Calibration Data

Console Data		Calibration Data		
No.	Serial No.	Date	y	ΔH_{g} (mmH ₂ O)
B01	1563	01/12/2025	1.003	49.79
B02	8002514	01/12/2025	1.004	49.61
B03	1503016	03/12/2025	0.999	49.84
B04	00006659	02/12/2025	0.998	50.06
B05	00007428	01/12/2025	1.005	49.40
R01	1561	01/12/2025	0.997	49.92
R02	8002513	03/12/2025	0.999	49.70
R03	1570	03/12/2025	1.002	49.82
R04	8002519	01/12/2025	1.005	49.95
R05	1503015	03/12/2025	0.998	49.86

Remark : Accept Value of y (test) is $0.97 < y < 1.03$

Accept Value of ΔH_{g} (test) is 46.7 ± 6.4 (mmH₂O)

Calibrated by :

Adul Dangklom

(Mr. Adul Dangklom)

Approved by :

Peera Detudom

(Mr. Peera Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด

S.P.S. CONSULTING SERVICE CO., LTD.

7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900

7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900

Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

Pitot Tube Calibration Report

Calibration Method

Standard Pitot Tube

Calibration Data

Pitot Tube Data			Calibration Data		
No.	Type of Pitot	Coefficient of Standard Pitot	Date	Avg. of Cp (test)	
				Side A	Side B
B36	S	0.99	03/11/2025	0.85	0.84
B37	S	0.99	03/11/2025	0.84	0.84
B38	S	0.99	03/11/2025	0.84	0.84
B39	S	0.99	06/11/2025	0.84	0.85
B40	S	0.99	06/11/2025	0.84	0.84
B41	S	0.99	04/11/2025	0.85	0.84
B44	S	0.99	03/11/2025	0.84	0.84
B45	S	0.99	03/11/2025	0.84	0.84
B46	S	0.99	03/11/2025	0.85	0.84
B47	S	0.99	04/11/2025	0.84	0.83
B48	S	0.99	04/11/2025	0.85	0.84
B49	S	0.99	04/11/2025	0.84	0.84
B54	S	0.99	05/11/2025	0.85	0.84
B56	S	0.99	05/11/2025	0.84	0.85
B57	S	0.99	05/11/2025	0.84	0.84
B58	S	0.99	04/11/2025	0.84	0.85

Remark : Accept value of Cp (test) is 0.84 ± 0.01

Calibrated by :

Adul Dangklom
(Mr. Adul Dangklom)


Approved by :

Peera Detudom
(Mr. Peera Detudom)



CALIBRATION LABORATORY Co.,LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-G353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



CERTIFICATE OF CALIBRATION FOR

NOMENCLATURE	VACUUM GAUGE
MANUFACTURER	HI-LIGHT
MODEL/TYPE	N/A
SERIAL NO.	N/A[64-220066-2]
CLID.NO.	212301420
JOB CONTROL NO.	240720076549

CUSTOMER S.P.S. CONSULTING SERVICE CO., LTD.
7 SOI PHAHOLYOTHIN 24 ROAD., JOMPOL,
CHATUCHAK, BANGKOK 10900


DATE OF RECEIVED : 19 July 2025

DATE OF ISSUED: 24 July 2025

The report or calibration shall not be reproduced except in full without approval of the Calibration Laboratory Co., Ltd.

Calibrated By : Sittipong Pimdee
Calibration Engineer

Approved By : Mongkol Yotsoontorn
Authorized Signatory
24 July 2025



This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to the International System of Units (SI)

Certificate No. Q24076549

F3-011-05/12-23

page 1 of 3



CALIBRATION LABORATORY Co., LTD.

211Q-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-Q353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



CALIBRATION AND
DIMENSIONAL MEASUREMENT
ACDM-2814

REPORT OF CALIBRATION

FOR

NOMENCLATURE	VACUUM GAUGE
MANUFACTURER	HI-LIGHT
MODEL/TYPE	N/A
SERIAL NO.	N/A [64-220066-2]
DATE OF CALIBRATION	23 July 2025
DUE DATE OF CALIBRATION	23 July 2026

ENVIRONMENT CONDITIONS

Temperature : $(23 \pm 2) ^\circ\text{C}$

Relative Humidity $(55 \pm 10) \% \text{RH}$

PROCEDURE USED :

This instrument was calibrated under procedure No. CLC-CPPP-05 according to DKD-R 6-1 as calibration guidelines.

The calibration was performed by direct measurement with Document Process Calibrator and Pressure Module which maintained by the Calibration Laboratory Co., Ltd.

REFERENCE STANDARD USED :

Document Process Calibrator, Fluke Model 74 1B *S/N.* 8295020 with Pressure Module Model 700PD5 *S/N.* 89404505.

TRACEABILITY :

The measurement s are traceable to International System of Units (SI), through National Institute of Metrology (Thailand).
Certificate No. MP-0040-24.

UNCERTAINTY :

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor of $k=2$. It has been evaluated according to the "Calibration of Pressure Gauges (DKD-R 6-1)" which provides a level of confidence approximately 95%.

Certificate No. Q24076549

F3-011-05/12-23

page 2 of 3

CONDITION OF CALIBRATION ITEM :RECEIVED IN GOOD OPERATIONAL CONDITION

MEASUREMENT RESULTS: (X) without adjustment () adjustment

The DUC was exercised by applying a known pressure from its zero to full scale 1 times. Then 2 series of known gauge pressure were applied. The STD reading were recorded and the means value were reported in the table below.

CALIBRATION DATA

CORRECTION OF PRESSURE

DUC Test point (inHg)	STD Reading (kPa)		Conversion to inHg		Correction (inHg)	
	Up	Down	Up	Down	Up	Down
0	0.00	0.00	0.0	0.0	0.0	0.0
-5	-17.61	-17.95	-5.2	-5.3	+0.2	+0.3
-10	-34.54	-34.54	-10.2	-10.2	+0.2	+0.2
-15	-51.13	-51.47	-15.1	-15.2	+0.1	+0.2
-20	-67.72	-68.06	-20.0	-20.1	+0.0	+0.1
-25	-84.31	-84.31	-24.9	-24.9	+0.1	+0.1
-30	-101.24	-101.24	-29.9	-29.9	+0.1	+0.1

Uncertainty of measurement ± 0.2 inHg

Transmitting fluid : Air.

Technical Note. Conversion factor 1 kPa ; 0.2953003 inHg

Note. The Scope of Accredited ANAB Certificate No. ACDM-2814 Version 012 Page 43 of 67

This report is valid for the above stated instrument/s only.

End of Certificate

Certificate No. Q24076549

F3-011-05/ 12-23



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด

S.P.S. CONSULTING SERVICE CO., LTD.

7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900

7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900

Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com., www.spscon.com

Personal Pump Calibration Report

Calibration Method : Dry Cal Primary Flowmeter

Model : Defender 510-H

S/N : 136164

Environmental Conditions

Temperature . 25 ± 3 °C
Pressure . 1010 ± 15 mmbar

Personal Pump Data				Calibration Data								
No.	Brand	Model	Serial No.	Date	Flow Rate (ml/min)						Value From Calibration Curve	
					Setting			Actual (Q std.)				
					1	2	3	1	2	3	y	R ²
B41	SKC	224-PCXR4	612669	01/10/2025	1,000	1,500	2,000	1,010	1,508	2,009	1.000x + 2.612	0.999
B42	SKC	224-PCXR4	626041	02/10/2025	1,000	1,500	2,000	1,004	1,494	1,994	0.997x + 1.344	1.000
B43	SKC	224-PCXR4	034636	01/10/2025	1,000	1,500	2,000	998	1,505	2,002	1.001x - 5.177	1.000
B44	SKC	224-PCXR8	529341	01/10/2025	1,000	1,500	2,000	999	1,496	1,998	0.996x + 0.909	1.000
B45	SKC	224-PCXR8	529594	01/10/2025	1,000	1,500	2,000	996	1,510	1,992	1.005x - 11.543	1.000
B46	SKC	224-PCXR8	566743	01/10/2025	1,000	1,500	2,000	1,003	1,488	1,997	0.994x + 3.717	1.000
B47	SKC	224-PCXR8	566747	01/10/2025	1,000	1,500	2,000	1,004	1,500	1,993	0.996x + 2.230	1.000
B48	SKC	224-PCXR8	566753	01/10/2025	1,000	1,500	2,000	1,002	1,501	1,991	1.000x - 4.116	0.999
B49	SKC	224-PCXR8	566780	01/10/2025	1,000	1,500	2,000	995	1,502	1,990	0.997x - 1.978	1.000
B50	SKC	224-PCXR8	500400	02/10/2025	1,000	1,500	2,000	997	1,503	2,001	1.004x - 10.178	1.000
B51	SKC	224-PCXR8	500363	01/10/2025	1,000	1,500	2,000	1,001	1,502	1,993	0.995x + 2.848	1.000
B52	SKC	224-PCXR8	093186	03/10/2025	1,000	1,500	2,000	996	1,510	1,999	1.005x - 12.252	0.999
B53	SKC	224-PCXR8	707670	03/10/2025	1,000	1,500	2,000	1,002	1,496	2,004	1.003x - 8.791	1.000
B54	SKC	224-PCXR3	509821	03/10/2025	1,000	1,500	2,000	999	1,501	1,995	0.999x - 2.090	1.000
B55	SKC	224-PCXR3	510710	02/10/2025	1,000	1,500	2,000	1,002	1,503	2,006	1.007x - 13.250	0.999
B56	SKC	224-PCXR3	511450	01/10/2025	1,000	1,500	2,000	995	1,505	1,997	1.002x - 7.594	1.000
B57	SKC	224-PCXR3	510798	02/10/2025	1,000	1,500	2,000	998	1,500	1,994	0.999x - 7.163	0.999
B58	SKC	224-PCXR3	509852	03/10/2025	1,000	1,500	2,000	1,002	1,494	1,996	0.993x + 6.485	1.000
B59	SKC	224-PCXR3	509862	01/10/2025	1,000	1,500	2,000	1,006	1,505	1,998	0.996x + 5.117	1.000
B60	SKC	224-PCXR3	512655	02/10/2025	1,000	1,500	2,000	1,004	1,501	2,003	1.010x - 14.223	0.999
B61	SKC	224-PCXR3	503915	03/10/2025	1,000	1,500	2,000	993	1,495	1,994	0.999x - 4.942	1.000
B62	SKC	224-PCXR3	505975	03/10/2025	1,000	1,500	2,000	995	1,500	2,005	1.009x - 16.396	1.000
B63	SKC	224-PCXR3	511432	03/10/2025	1,000	1,500	2,000	996	1,497	1,991	0.998x - 3.171	1.000
B64	SKC	224-PCXR3	508302	03/10/2025	1,000	1,500	2,000	1,008	1,506	1,998	0.992x + 8.667	0.999
B65	SKC	224-PCXR3	508310	03/10/2025	1,000	1,500	2,000	1,006	1,492	2,003	1.000x - 4.355	1.000
B66	SKC	224-PCXR3	509861	03/10/2025	1,000	1,500	2,000	994	1,496	1,994	0.997x - 0.275	1.000
B67	SKC	224-PCXR3	506295	01/10/2025	1,000	1,500	2,000	997	1,505	2,001	1.004x - 10.258	1.000
B68	SKC	224-PCXR3	505872	03/10/2025	1,000	1,500	2,000	998	1,512	1,992	0.999x - 3.554	0.999
B69	SKC	224-PCXR3	508375	01/10/2025	1,000	1,500	2,000	997	1,489	1,996	0.997x - 2.309	1.000
B70	SKC	224-PCXR3	510623	03/10/2025	1,000	1,500	2,000	1,001	1,496	1,991	0.992x + 7.131	1.000
B71	SKC	224-PCXR3	508367	03/10/2025	1,000	1,500	2,000	999	1,498	1,995	0.994x + 6.433	1.000
B72	SKC	224-PCXR3	505977	03/10/2025	1,000	1,500	2,000	996	1,507	1,999	1.003x - 7.490	1.000
B73	SKC	224-PCXR3	512606	03/10/2025	1,000	1,500	2,000	1,004	1,503	2,003	1.001x - 5.285	0.999
B74	SKC	224-PCXR3	505993	01/10/2025	1,000	1,500	2,000	1,006	1,501	1,997	0.993x + 8.232	1.000
B75	SKC	224-PCXR3	509820	02/10/2025	1,000	1,500	2,000	1,005	1,494	1,995	0.997x - 2.979	0.999
B76	SKC	224-PCXR3	509811	02/10/2025	1,000	1,500	2,000	996	1,503	1,999	1.005x - 10.613	1.000
B77	SKC	224-PCXR3	508301	01/10/2025	1,000	1,500	2,000	1,003	1,490	1,998	0.994x + 4.694	1.000
B78	SKC	224-PCXR3	510677	01/10/2025	1,000	1,500	2,000	1,004	1,492	1,997	0.995x + 4.036	1.000
B79	SKC	224-PCXR3	510920	01/10/2025	1,000	1,500	2,000	1,008	1,504	2,006	1.006x - 9.588	0.999

Calibrated by :

Adul Dangklom
(Mr. Adul Dangklom)

Approved by :

Peera Detudom
(Mr. Peera Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

Personal Pump Calibration Report

Calibration Method : Dry Cal Primary Flowmeter

Model : Defender 510-H

S/N : 136833

Environmental Conditions

Temperature : 25 $\pm$ 3 $^{\circ}$ C
Pressure : 1010 $\pm$ 15 mmbar

Personal Pump Data				Calibration Data								
No.	Brand	Model	Serial No.	Date	Flow Rate (ml/min)						Value From Calibration Curve	
					Setting			Actual (Q std.)			y	R ²
					1	2	3	1	2	3		
R01	SKC	224-PCXR4	602467	01/10/2025	1,000	1,500	2,000	1,001	1,504	2,006	1.001x + 1.123	1.000
R02	SKC	224-PCXR4	626450	01/10/2025	1,000	2,000	3,000	997	1,511	1,997	1.000x - 2.215	1.000
R03	SKC	224-PCXR4	691592	01/10/2025	1,000	1,500	2,000	1,004	1,504	2,008	1.005x - 5.705	1.000
R04	SKC	224-PCXR4	691672	01/10/2025	1,000	1,500	2,000	1,013	1,505	2,007	0.996x + 7.748	0.999
R05	SKC	224-PCXR4	798470	01/10/2025	1,000	1,500	2,000	1,005	1,506	2,010	1.007x - 4.757	1.000
R06	SKC	224-PCXR4	798456	01/10/2025	1,000	1,500	2,000	996	1,503	1,999	1.003x - 5.913	1.000
R07	SKC	224-PCXR4	798480	03/10/2025	1,000	1,500	2,000	997	1,502	1,996	1.000x - 8.975	0.999
R08	SKC	224-PCXR4	883215	03/10/2025	1,000	1,500	2,000	1,005	1,504	1,995	0.999x - 0.068	1.000
R09	SKC	224-PCXR4	034650	03/10/2025	1,000	1,500	2,000	994	1,505	1,998	1.005x - 11.989	1.000
R10	SKC	224-PCXR4	091765	01/10/2025	1,000	1,500	2,000	1,005	1,508	2,006	1.008x - 11.738	0.999
R11	SKC	224-PCXR4	091763	01/10/2025	1,000	1,500	2,000	1,006	1,493	2,003	0.996x + 5.589	1.000
R12	SKC	224-PCXR4	091568	02/10/2025	1,000	1,500	2,000	995	1,496	1,999	1.002x - 5.717	1.000
R13	SKC	224-PCXR4	091638	01/10/2025	1,000	1,500	2,000	1,012	1,505	2,008	1.004x - 2.938	0.999
R14	SKC	224-PCXR4	091764	01/10/2025	1,000	1,500	2,000	996	1,494	2,004	1.008x - 18.690	1.000
R15	SKC	224-PCXR8	529457	01/10/2025	1,000	1,500	2,000	998	1,507	2,007	1.007x - 12.957	0.999
R16	SKC	224-PCXR8	529643	01/10/2025	1,000	1,500	2,000	997	1,496	1,994	0.999x - 1.395	1.000
R17	SKC	224-PCXR8	529645	01/10/2025	1,000	1,500	2,000	1,005	1,503	1,995	1.005x - 10.886	0.999
R18	SKC	224-PCXR8	566756	01/10/2025	1,000	1,500	2,000	997	1,505	1,993	1.000x - 4.450	1.000
R19	SKC	224-PCXR8	566802	01/10/2025	1,000	1,500	2,000	1,004	1,504	2,007	1.006x - 6.752	1.000
R20	SKC	224-PCXR8	529089	03/10/2025	1,000	1,500	2,000	1,008	1,497	2,001	1.002x - 6.225	0.999
R21	SKC	224-PCXR8	665728	03/10/2025	1,000	1,500	2,000	997	1,505	2,003	1.006x - 16.975	0.999
R22	SKC	224-PCXR8	707444	01/10/2025	1,000	1,500	2,000	1,005	1,494	2,001	0.995x + 6.369	1.000
R23	SKC	224-PCXR8	761067	01/10/2025	1,000	1,500	2,000	1,008	1,495	2,000	0.992x + 13.025	1.000
R24	SKC	224-PCXR8	707893	01/10/2025	1,000	1,500	2,000	1,005	1,504	1,997	1.004x - 8.140	0.999
R25	SKC	224-PCXR8	761052	01/10/2025	1,000	1,500	2,000	1,006	1,510	2,006	1.001x - 0.152	0.999
R26	SKC	224-PCXR8	707956	01/10/2025	1,000	1,500	2,000	1,000	1,513	2,008	1.008x - 10.714	1.000
R27	SKC	224-PCXR8	707398	02/10/2025	1,000	1,500	2,000	1,011	1,512	2,012	1.002x + 2.547	0.999
R28	SKC	224-PCXR8	707481	02/10/2025	1,000	1,500	2,000	999	1,498	2,000	1.000x + 0.144	1.000
R29	SKC	224-PCXR8	707402	02/10/2025	1,000	1,500	2,000	1,000	1,509	2,006	1.004x - 5.501	1.000
R30	SKC	224-PCXR8	093811	02/10/2025	1,000	1,500	2,000	998	1,514	2,005	1.009x - 10.222	1.000
R31	SKC	224-PCXR8	093183	01/10/2025	1,000	1,500	2,000	999	1,508	2,003	1.005x - 9.587	1.000
R32	SKC	224-PCXR8	671950	01/10/2025	1,000	1,500	2,000	1,000	1,494	1,996	0.994x + 5.137	1.000
R33	SKC	224-PCXR4	626254	01/10/2025	1,000	1,500	2,000	1,004	1,493	2,005	1.008x - 16.151	0.999
R34	SKC	224-PCXR4	626131	01/10/2025	1,000	1,500	2,000	998	1,508	1,994	0.998x - 0.764	1.000
R35	SKC	224-PCXR8	707460	01/10/2025	1,000	1,500	2,000	1,003	1,502	1,993	0.993x + 8.172	1.000
R36	SKC	224-PCXR8	707446	01/10/2025	1,000	1,500	2,000	997	1,510	1,999	1.004x - 8.044	1.000
R37	SKC	224-PCXR8	707432	01/10/2025	1,000	1,500	2,000	1,012	1,515	2,007	0.997x + 7.376	0.999
R38	SKC	224-PCXR8	707349	03/10/2025	1,000	1,500	2,000	999	1,511	1,998	1.001x - 2.918	1.000
R39	SKC	224-PCXR8	761095	03/10/2025	1,000	1,500	2,000	1,008	1,514	1,996	0.993x + 11.058	0.999

Calibrated by :

Adul Dangklom
(Mr. Adul Dangklom)

Approved by :

(Mr. Peera Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com., www.spscon.com

Personal Pump Calibration Report

Calibration Method : Dry Cal Primary Flowmeter

Model : Defender 510-H

S/N : 136833

Environmental Conditions

Temperature : 25 $\pm$ 3 $^{\circ}$ C
Pressure : 1010 $\pm$ 15 mmbar

Personal Pump Data				Calibration Data								
No.	Brand	Model	Serial No.	Date	Flow Rate (ml/min)						Value From Calibration Curve	
					Setting			Actual (Q std.)			y	R ²
					1	2	3	1	2	3		
R40	SKC	224-PCXR4	612753	03/10/2025	1,000	1,500	2,000	1,005	1,504	2,007	1.003x - 2.699	1.000
R41	SKC	224-PCXR4	626140	03/10/2025	1,000	1,500	2,000	998	1,498	2,000	1.001x - 1.631	1.000
R42	SKC	224-PCXR4	626463	03/10/2025	1,000	1,500	2,000	1,004	1,496	1,999	0.993x + 9.615	1.000
R43	SKC	224-PCXR4	626129	03/10/2025	1,000	1,500	2,000	1,002	1,505	2,003	1.008x - 13.761	0.999
R44	SKC	224-PCXR4	602753	01/10/2025	1,000	1,500	2,000	1,004	1,503	1,999	1.006x - 9.411	0.999
R45	SKC	224-PCXR4	626137	01/10/2025	1,000	1,500	2,000	997	1,504	1,998	1.002x - 3.862	1.000

Calibrated by :

Adul Dangklom
(Mr. Adul Dangklom)

Approved by :

Peera Detudom
(Mr. Peera Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com.. www.spscon.com

Rotameter Calibration Report (For Personal Pump High Flow Adjust)

Calibration Method : Dry Cal Primary Flowmeter

Model : Defender 510-H

S/N : 136833

Calibration Data

Calibration Data											
Rotameter Data			Calibration Data								
No.	Brand	Model	Date	Flow Rate (mL/min)						Value From Calibration Curve	
				Flow Rate (Reading)			Actual (Q std.)				
				1	2	3	1	2	3	y	R ²
H-R01	Dwyer	VFB-65	01/10/2025	500	1,000	2,000	501.1	997.7	1996.7	1.000x - 2.348	0.999
H-R02	Dwyer	VFB-65	01/10/2025	500	1,000	2,000	500.3	999.2	1997.5	1.001x - 2.181	1.000
H-R03	Dwyer	VFB-65	02/10/2025	500	1,000	2,000	500.9	1001.1	1999.3	0.999x + 0.708	0.999
H-R04	Dwyer	VFB-65	02/10/2025	500	1,000	2,000	501.4	999.4	1998.9	0.997x + 3.139	1.000
H-R05	Dwyer	VFB-65	01/10/2025	500	1,000	2,000	500.5	1000.7	1998.2	0.998x + 2.480	1.000
H-R06	Dwyer	VFB-65	03/10/2025	500	1,000	2,000	502.0	998.5	1994.8	1.000x - 1.968	0.999

Calibrated by :

Adul Dangklom
(Mr.Adul Dangklom)

Approved by :

Peera Detudom
(Mr. Peera Detudom)



CERTIFICATE No : 25M2254

REFERENCE No : 76365-1

PAGE : 1 OF 2

Certificate of Calibration

EQUIPMENT : DIGITAL BALANCE

MANUFACTURER : METTLER TOLEDO

MODEL : XS105DU

SERIAL No : 1126422905


ID No : BA05/50

CONDITION AS RECEIVED : USED ITEM

SUBMITTED BY : S.P.S. CONSULTING SERVICE CO., LTD.
7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN RD.,
JOMPOL, CHATUCHAK, BANGKOK 10900

CALIBRATED BY : ATSAWIN Y.

CALIBRATION DATE : 07-Mar-25

APPROVED BY : 
PONGSAK J.

ISSUED DATE : 13-Mar-25

RECEIVED DATE : 07-Mar-25

THIS CERTIFICATE MAY NOT BE REPRODUCED OTHER THAN IN FULL EXCEPT WITH THE PRIOR WRITTEN APPROVAL OF
QUALITY CALIBRATION CO., LTD.





CERTIFICATE No : 25M2254

PAGE : 2 OF 2

Calibration Report

EQUIPMENT : DIGITAL BALANCE MODEL : XS105DU
MANUFACTURER : METTLER TOLEDO S/N : 1126422905
ID No : BA05/50 RECEIVED DATE : 07-Mar-25
AIR PRESSURE : 1009mbar $\pm$ 1mbar CALIBRATION DATE : 07-Mar-25
AMBIENT TEMPERATURE : 24° C $\pm$ 1° C RELATIVE HUMIDITY : 54 %RH $\pm$ 10 % RH

CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED BY ACCORDING TO UKAS LAB 14 EDITION 6:2019 BY USING KNOWN WEIGHT STANDARD WEIGHT. THE BALANCE WAS NOT ADJUSTED BEFORE CALIBRATION. THE BALANCE HAS NO ZERO TRACKING FUNCTION. REPEATABILITY WAS MEASURED BY USING 10 REPEATED MEASUREMENTS. LINEARITY WAS MEASURED COVERING 10 POINTS, EVENLY SPREAD OVER THE RANGE. THE INSTRUMENT WAS SET ZERO BEFORE PERFORMING THE LINEARITY TEST. OFF-CENTER LOADING WAS MEASURED BY USING STANDARD WEIGHTS PLACED ON THE PAN AND MOVED TO VARIOUS POSITIONS ON THE PAN.

2. REFERENCE STANDARD INSTRUMENTS :-

<u>INSTRUMENT</u>	<u>MODEL</u>	<u>SERIAL No</u>	<u>CERTIFICATE No</u>	<u>DUE DATE</u>
1) STANDARD WEIGHT SET	E2	QK-I-151	C02250116	28-Jan-27
2) STANDARD WEIGHT	E2	15843	C02250117	29-Jan-27

3. THE CERTIFICATE IS VALID FOR THE ITEM CALIBRATED AS SHOWN ON THE DATE AND PLACE OF CALIBRATION ONLY.

4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.

5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-

- NATIONAL INSTITUTE OF METROLOGY (THAILAND)

RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

1. ZERO SETTING FUNCTION : NORMAL


2. TARE FUNCTION : NORMAL

3. REPEATABILITY OF READING AT 120 g WAS 0.000055 g

4. DEPARTURE FROM NOMINAL VALUE/ LINEARITY

NOMINAL VALUE (g)	BALANCE READING (g)	CORRECTION (g)	UNCERTAINTY ($\pm$ g)
0.00	0.00000	0.00000	0.000065
0.02	0.01999	0.00001	0.000065
0.10	0.10001	-0.00001	0.000066
0.20	0.20001	-0.00001	0.000066
0.50	0.50002	-0.00002	0.000065
1.00	1.00003	-0.00003	0.000066
2.00	2.00001	-0.00001	0.000067
5.00	5.00002	-0.00002	0.000068
10.00	10.00000	0.00000	0.000070
20.00	20.00004	-0.00004	0.000078
50.00	50.00000	0.00000	0.00013
100.00	100.0001	-0.0001	0.00019
120.00	120.0002	-0.0002	0.00022

5. OFF CENTER LOADING ERROR



POINT	READING (g)
1	50.0000
2	50.0000
3	50.0000
4	50.0000
5	50.0000
OFF-CENTER LOADING	0.0000

NOTE: THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA
THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR $k=2$, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT



SITHIPORN ASSOCIATES CO., LTD.
CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbunru, Bangplud, Bangkok, 10700 Thailand
Tel. +66 2433 8331 Email : calibration@sithiporn.com

SITHIPORN
associates



Cert. No. : SP25026

Pages : 1 of 4

Calibration Certificate

Equipment : UV-VIS SPECTROPHOTOMETER
Manufacturer : PERKINELMER
Model : LAMBDA 25
Serial No.: 501S14123010
ID No.: SP03/58
Calibration Mode : WAVELENGTH ACCURACY
PHOTOMETRIC ACCURACY
STRAY LIGHT

Condition As Found : GOOD

Customer : S.P.S CONSULTING SERVICE CO., LTD.
7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN ROAD,
CHOMPHON SUB-DISTRICT, CHATUCHAK DISTRICT,
BANGKOK PROVINCE 10900 THAILAND.

Location : ORGANIC LABORATORY IV

Ambient Temperature : (22.9 $\pm$ 5) °C
Relative Humidity : (53.7 $\pm$ 25) %

Received Date : 22 AUGUST 2025
Calibration Date : 22 AUGUST 2025
Date of Issue : 25 AUGUST 2025

Calibrated by :

Nitinun Srihawan

Approved by :

Wichok B.
(Wichok Ekpongpradit)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

Cert. No. : SP25026

Job No. : VC68SP0019

Pages : 2 of 4

Calibration Method :

This instrument was calibrated by using on-site calibration procedure In-house method : CP-SP-01

The calibration procedure to direct measurement wavelength accuracy by using wavelength standard solution, Photometric accuracy by using absorbance standard filter and absorbance standard solution

The calibration procedure used was based on ASTM E275-01, ASTM E925-02

Condition of this result of calibration :

1. Certified reference materials

<u>Material</u>	<u>Ref. type</u>	<u>Cell serial No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
Holmium liquid	RM-HL	29706	126461	24/10/2026
Didymium liquid	RM-DL	28912	126462	24/10/2026
Neutral density filter	RM-1N2N3N	13877	126457	24/10/2026
Potassium dichromate solutions	RM-0204060810	14204	126497	25/10/2026
Potassium Iodide solution	-	KI-0701-001	CI-0185-24	14/05/2026

2. This result of calibration was found accurate as shown on date and place of calibration only.

3. This certificate is traceable to the international system of unit maintained at :

3.1 The UK National Physical Laboratory (NPL)

Result of calibration : Wavelength Accuracy

(Without adjustment)

Material	Certified Values of Reference Material (nm)	UUC* Reading (nm)	Error (nm)	Uncertainty ± (nm)	k Factor
RM-HL	278.13	278.21	0.08	0.16	2.00
	361.25	361.39	0.14	0.16	2.00
	467.82	467.71	-0.11	0.16	2.00
	536.56	536.50	-0.06	0.16	2.00
	640.50	640.36	-0.14	0.16	2.00
RM-DL	740.09	739.85	-0.24	0.16	2.00
	864.94	865.12	0.18	0.16	2.00

UUC* = Unit Under Calibration

Cert. No. : SP25026
Job No. : VC68SP0019
Pages : 3 of 4

Result of calibration : Photometric Accuracy

Material	Wavelength (nm)	Filter S/N	Nominal Absorbance (A)	Certified Absorbance (A)	UUC* Reading Absorbance (A)	Error (A)	Uncertainty ± (A)	k Factor
Neutral Density glass filter	440.0	29381	0.5	0.5443	0.5413	-0.0030	0.0043	2.00
		29914	0.7	0.7484	0.7455	-0.0029	0.0054	2.00
		29360	1.0	1.0527	1.0535	0.0008	0.0032	2.00
	465.0	29381	0.5	0.4948	0.4922	-0.0026	0.0041	2.00
		29914	0.7	0.6906	0.6877	-0.0029	0.0050	2.00
		29360	1.0	0.9695	0.9709	0.0014	0.0031	2.00
	546.1	29381	0.5	0.5090	0.5068	-0.0022	0.0036	2.00
		29914	0.7	0.6985	0.6960	-0.0025	0.0041	2.00
		29360	1.0	0.9814	0.9825	0.0011	0.0031	2.00
	590.0	29381	0.5	0.5375	0.5353	-0.0022	0.0034	2.00
		29914	0.7	0.7256	0.7231	-0.0025	0.0037	2.00
		29360	1.0	1.0213	1.0219	0.0006	0.0032	2.00
	635.0	29381	0.5	0.5223	0.5202	-0.0021	0.0033	2.00
		29914	0.7	0.6927	0.6901	-0.0026	0.0036	2.00
		29360	1.0	0.9744	0.9750	0.0006	0.0032	2.00

UUC* = Unit Under Calibration

Cert. No. : SP25026
Job No. : VC68SP0019
Pages : 4 of 4

Result of calibration : Photometric Accuracy

(Without adjustment)

Material	Wavelength (nm)	Solution (mg/l)	Certified Absorbance (A)	UUC* Reading Absorbance (A)	Error (A)	Uncertainty ± (A)	k Factor
Potassium dichromate solutions	235.0	20	0.2415	0.2443	0.0028	0.0101	2.00
		40	0.4866	0.4871	0.0005	0.0115	2.00
		60	0.7415	0.7295	-0.0120	0.0067	2.00
		80	0.9854	0.9844	-0.0010	0.0071	2.00
		100	1.2444	1.2425	-0.0019	0.0073	2.00

UUC* = Unit Under Calibration

Condition of this result of calibration : Spectrophotometer PERKINELMER Model LAMBDA 25 S/N 501S14123010

Resolution of Wavelength Mode 0.1 nm

Resolution of Photometric Mode 0.001 A

Parameter Setting

Measurement Mode Wavelength, Absorbance

Wavelength Scan 190 nm - 1100 nm

Scanning Speed 7.5 nm/min

Band width(Wavelength) 1.0

Band width(Vis) 1.0

Band width(Uv) 1.0

Stray Light** UUC* Reading at 220.0 nm	
Transimission T(%)	Absorbance(A)
0.020	3.7032

**Specific Acceptance :

Transmission ≤ 1.0 T(%), Absorbance ≥ 2.0 A

**Stray light not TISI Accredited

The reported uncertainty is based on a standard uncertainty multiplied by a coverage factor k , providing a level of confidence of approximately 95%

End of Calibration Certificate



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด

S.P.S. CONSULTING SERVICE CO., LTD.

7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900

7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900

Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

Calibration Report					
Non-Dispersive Infrared CO Analyzer					
Date :	01 December 2025	Brand :	API	Model :	300E
No.	CO-B02			Serial No.	965
Calibrator (Dilution System)					
Brand : API			Model : 700		
Last Cal. Date : 01 September 2025			Serial No. : 911		
Reference Standard Gas					
Standard Gas : Carbon Monoxide (CO)			Cylinder No. : D711839		
Certified Date : 14 March 2024		Expired Date : 14 March 2032		Cylinder Conc. : 4,580 ppm	
Calibrating Condition					
Pressure : 1011 mmbar		Temp. : 24.6 °C		% RH : 50	
Calibration Setting					
Span	Initial Reading (Before Adj.), PPM			Final Reading (After Adj.), PPM	
Set Point	Expected Concentration	Analyzer Response		%Dif	
Zero	0	-0.10		-	
CO Span	40.00	39.94		-0.150	
API Model 300E CO Analyzer Check List					
Parameter	Observed Value	Units	Nominal Range		
Range	50	PPM	0-1000 ppm		
Stability	0.10	PPM	< 1 ppm With Zero Air		
CO Measure	4017.2	mV	2500-4800 mV		
CO Reference	3948.8	mV	2500-4800 mV		
Measure/Reference Ratio	1.180	-	1.1-1.3 W/Zero Air		
Sample Pressure	28.5	In-Hg-A	~2" < Ambient Absolute Pressure		
Sample Flow	810	CC/Min	800 ± 10%		
Sample Temperature	48.2	°C	48 ± 4		
Bench Temperature	48.0	°C	48 ± 2		
Wheel Temperature	68.5	°C	68 ± 2		
Box Temperature	30.6	°C	Ambient Temp + 7 ± 10		
Photo-Drive	3034.9	mV	250 mV to 4750 mV		
Slope	1.017	-	1.0 ± 0.3		
Offset	0.2	-	0 ± 0.3		

Calibrated by :

Adul Dangklom
(Mr.Adul Dangklom)

Approved by :

Peera Detudom
(Mr. Peera Detudom)



MAINTENANCE AND TEST CERTIFICATE MODEL

OPTIMA 5300DV

Customer : <u>S.P.S.Consulting Service Co.,Ltd</u>	Date Tested: <u>July 1, 2025</u>	
	Recommendation Recertification	
Address : <u>7 Soi Phaholyothin 24</u>	Period <u>6</u> Months	
<u>Paholyothin Road</u>	Recertification Due: <u>January 1, 2026</u>	
<u>Jompol Chatuchak, Bangkok 1090</u>	Date Last Certified: <u>January 6, 2025</u>	
User Name: <u>K.Phenpha Vipasthawatt</u>	Visit Number: <u>1 of 2</u>	
Phone: <u>083-9269252</u>	PerkinElmer Phone: <u>02-719-6420 ext 206</u>	
Fax: <u>02-513-4221</u>	PerkinElmer Fax: <u>02-318-5597</u>	

CONFIGURATION TESTED		ACCESSORIES/COMPONENT NOT INCLUDED
MODEL	SERIAL NUMBER	
<u>OPTIMA 5300DV</u>	<u>077C7042401</u>	
TESTED EQUIPMENT	CALIBRATION NUMBER	EXPIRATION
<u>IPV Methods</u>		
TEST STANDARD USED	PART NUMBER	EXPIRATION DATE
<u>Multielement Standard</u>	<u>N069-1579</u>	<u>December 30, 2024</u>
<u>Wavecal Solution</u>	<u>N058-2152</u>	<u>March 30, 2024</u>
<u>VIS Wavecal solution</u>	<u>N930-2946</u>	<u>February 28, 2024</u>
<u>Instrument Cal. STD4</u>	<u>N930-0221</u>	<u>November 30, 2024</u>
CUSTOMER SUPPLIED	COMMENTS	CUSTOMER INITIALS
<u>2 % HNO3</u>		
<u>10 % HNO3</u>		



MAINTENANCE AND TEST CERTIFICATE MODEL

OPTIMA 5300DV

SERIAL NUMBER 077C7042401
DATE TESTED July 1, 2025
1. MECHANICAL CHECKS

A. Inspect and clean all fans and filters.

☐ OK

B. Inspect and replace as necessary, all torch components including the RF coil.

☐ OK

C. Inspect all tubing for sign of clacking or leaking.

☐ OK

D. Adjust water and gas pressure regulator settings.

☐ OK

E. Inspect and leak check pneumatics drawers.

☐ OK

F. Clean the exterior of the instrument.

☐ OK

2. OPTICAL CHECKS

A. Inspect and clean all optical components.

☐ OK

B. As required, check and replace all purgefilters.

☐ OK

C. Recheck optical alignment.

☐ OK

3. COOLING SYSTEM CHECKS

A. Perform preventive maintenance on chiller.

☐ OK

B. Flush out the chiller every year.

☐ N/A

4. PERFORMANCE CHECKS

A. Torch View Alignment.

☐ OK

B. Wavelength Calibration.

☐ OK



MAINTENANCE AND TEST CERTIFICATE MODEL

OPTIMA 5300DV

SERIAL NUMBER : 077C7042401
DATE TESTED : July 1, 2025

PARAMETER		SPECIFICATION		FINAL VALUE	
Spectral Resolution : UV	As 193.696 nm	≤ 0.007		<u>0.00570</u>	
	Ni 231.604 nm	≤ 0.008		<u>0.00734</u>	
	Ni 341.476 nm	≤ 0.012		<u>0.00763</u>	
Spectral Resolution : VIS	La 408.672 nm	≤ 0.020		<u>0.01627</u>	
	Ba 455.403 nm	≤ 0.025		<u>0.02428</u>	
Precision					
	As 193.656 nm	% RSD	< 1.0	<u>0.82</u>	%
	Zn 213.856 nm	% RSD	< 1.0	<u>0.83</u>	%
	Mn 257.610 nm	% RSD	< 1.0	<u>0.20</u>	%
	La 379.478 nm	% RSD	< 1.0	<u>0.89</u>	%
	Ba 455.403 nm	% RSD	< 1.0	<u>0.92</u>	%
	Ba 493.408 nm	% RSD	< 1.0	<u>0.75</u>	%
Detection Limits : Axial	Tl 190.080 nm	3(sd)		<u>10.65</u>	ppb
	As 193.696 nm	3(sd)		<u>2.48</u>	ppb
	Pb 220.353 nm	3(sd)		<u>3.09</u>	ppb
Detection Limits : Radial	As 193.696 nm	3(sd)		<u>331.50</u>	ppb
	Zn 213.856 nm	3(sd)		<u>0.98</u>	ppb
	Mn 257.610 nm	3(sd)		<u>0.34</u>	ppb
	La 379.478 nm	3(sd)		<u>2.54</u>	ppb
	Ba 455.403 nm	3(sd)		<u>2.19</u>	ppb
	Ba 493.408 nm	3(sd)		<u>4.32</u>	ppb
BEC : Axial (IB X 500)/(IS-IB)	Cd 226.502 nm	≤ 150 ppb		<u>140.03</u>	
BEC : Radial (IB X 1000)/(IS-IB)	Mn 257.610 nm	≤ 45 ppb		<u>24.17</u>	



MAINTENANCE AND TEST CERTIFICATE MODEL
OPTIMA 5300DV

SERIAL NUMBER 077C7042401

DATE TESTED July 1, 2025

Remarks :

Commissioning follow as commissioning performance sheets.

This is to certify that the above tests have been performed and the configuration tested



meets




does not meet

the PerkinElmer Specifications listed on this certificate.

This certificate does not modify PerkinElmer's standard terms and condition of sale,
including warranty terms.

Service Department PerkinElmer Ltd.

Authorized Representative:



(Wiphan Promlumda)

Service Engineer

MAINTENANCE REPORT AND CALIBRATION CERTIFICATE

FLOW INJECTION MERCURY SYSTEMS MODEL

FIAS 100

Customer :	<u>S.P.S.Consulting Service Co.,Ltd</u>	Date Tested:	<u>July 1, 2025</u>
		Recommendation Recertification	
Address :	<u>7 Soi Phaholyothin 24</u>	Period	<u>6</u> Months
	<u>Paholyothin Road</u>	Recertification Due:	<u>January 1, 2026</u>
	<u>Jompol Chatuchak, Bangkok 10900</u>	Date Last Certified:	<u>January 6, 2025</u>
User Name:	<u>K.Phenpha Viphashtawat</u>	Visit Number:	<u>1 of 2</u>
Phone:	<u>083-9269252</u>	PerkinElmer Phone:	<u>02-719-6420 ext 8</u>
Fax:	<u>02-513-4221</u>	PerkinElmer Fax:	<u>02-318-5597</u>

CONFIGURATION TESTED

MODEL	SERIAL NUMBER	SOFTWARE
<u>FIAS 100</u>	<u>100S14090404</u>	<u>Syngistix version 7.3</u>
<u> </u>	<u> </u>	<u> </u>
<u> </u>	<u> </u>	<u> </u>
<u> </u>	<u> </u>	<u> </u>
<u> </u>	<u> </u>	<u> </u>

TEST STANDARD USED	PART NUMBER	EXPIRATION DATE
<u>Mercury (Hg) Std</u>	<u>N9300174</u>	<u>JUN 30, 2026</u>
<u> </u>	<u> </u>	<u> </u>
<u> </u>	<u> </u>	<u> </u>

MAINTENANCE REPORT AND CALIBRATION CERTIFICATE

FLOW INJECTION MERCURY SYSTEMS MODEL

FIAS 100

SERIAL NUMBER 100S14090404

DATE TESTED July 1, 2025

1. INSTRUMENT CHECKS

A. The light part, quartz windows and detector. Clean if necessary.

☐ OK

B. Inspect the mercury lamp. Alignment if necessary.

☐ OK

C. Inspect the mercury filter. Replace if necessary.

☐ OK

D. Inspect and clean or replace the dust filter.

☐ OK

E. Inspect peristaltic pump tubes. Replace if necessary.

☐ OK

2. ELECTRONICS CHECKS

A. Electronic power supplies

+ 5 Volts (± 0.3)

+ 4.98 Volts

+ 15 Volts (± 1.0)

+ 15.03 Volts

- 15 Volts (± 1.0)

- 15.07 Volts

+ 40 Volts (± 1.0)

+ 40.02 Volts

3. GAS SYSTEM CHECK

A. Leak test all internal and external gas box joints.

☐ OK

B. Inspect solenoid valve and pressure switch.

☐ OK

C. Inspect non return valve. Replace sleeve if necessary.

☐ OK

D. Inspect flow meter and needle valve. Clean if necessary.

☐ OK

4. MECHANICAL CHECKS

A. Inspect pump motor and pump roller.

☐ OK

B. Inspect and clean switching valve.

☐ OK

C. Inspect, clean and lubricant autosample.

☐ OK

MAINTENANCE REPORT AND CALIBRATION CERTIFICATE

FLOW INJECTION MERCURY SYSTEMS MODEL

FIAS 100

SERIAL NUMBER	<u>100S14090404</u>	DATE TESTED	<u>July 1, 2025</u>
PARAMETER		SPECIFICATION	ACTUAL VALUE
5. PERFORMANCE TEST			
A. Baseline Noise Test			
(measure peak area at 10 replicates without any sample)			
	SD	$\leq 0.0015 \text{ A*s}$	<u>0.0025</u> A*s
B. Sensitivity Check			
(10 ppb Hg Standard at 11 replicates)			
	Mean Absorbance	$\geq 0.0800 \text{ Abs.}$	<u>0.1201</u> Abs.
C. Characteristic mass(m_0)			
(10 ppb Hg Standard at 11 replicates)			
	m_0	$\leq 314 \text{ pg}$	<u>183.2</u> pg/0.0044A
D. Precision Check (%RSD)			
(10 ppb Hg Standard at 11 replicates)			
	%RSD	$\leq 2.5 \%$	<u>1.65</u> %

MAINTENANCE REPORT AND CALIBRATION CERTIFICATE

FLOW INJECTION MERCURY SYSTEMS MODEL

FIAS 100

SERIAL NUMBER 100S14090404**DATE TESTED** July 1, 2025

Remarks :

This is to certify that the above tests have been performed and the configuration tested



meets




does not meet

the PerkinElmer Specifications listed on this certificate.

This certificate does not modify PerkinElmer's standard terms and condition of sale,
including warranty terms.

Service Department PerkinElmer Ltd.

Customer Service Engineer:



(

Wiphan Promlumda

)

Service Engineer

คุณภาพน้ำ

CERTIFICATE OF CALIBRATION FOR

NOMENCLATURE : pH METER
MANUFACTURER : HANNA
MODEL / TYPE : HI3512/HI1332/HI7662-T
SERIAL NO. : 08685754/11250B7M/092806BN[PH04/56]
CLID. NO. : 272501562
JOB CONTROL NO. : 250617070523
CALIBRATION SERVICE : ☒ IN-LABORATORY ☐ ON-SITE

CUSTOMER : S.P.S. CONSULTING SERVICE CO., LTD.
7 SOI PHAHOLYOTHIN 24 ROAD, JOMPOL,
CHATUCHAK, BANGKOK 10900

DATE OF RECEIVED : 17 June 2025


DATE OF ISSUED : 20 June 2025

The report of calibration shall not be reproduced except in full without approval of the Calibration Laboratory Co., Ltd.

Calibrated By : Sukgasem Seehanart
Wenick Inchaisri
Calibration Engineer



Approved By : Mongkol Yotsoontorn
Authorized Signatory
20 June 2025



This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to
the International System of Units (SI)

Certificate No. Q25070523

F3-011-05/12-23

page 1 of 4






CLC
Accredited
ISO/IEC 17025

CALIBRATION LABORATORY Co., LTD.

2/10-11,14, 55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230

Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



REPORT OF CALIBRATION

FOR

NOMENCLATURE : **pH METER**
MANUFACTURER : **HANNA**
MODEL / TYPE : **HI3512/HI1332/HI7662-T**
SERIAL NO. : **08685754/11250B7M/092806BN[PH04/56]**
DATE OF CALIBRATION : **18 June 2025**

ENVIRONMENT CONDITIONS :

Temperature : **$(25 \pm 2.5) ^\circ\text{C}$**

Relative Humidity : **$(50 \pm 15) \% \text{ RH}$**

PROCEDURE USED :

This instrument was calibrated under procedure No. **CLC-CPCH-01** [pH Meter]. The calibration was performed by direct measurement with Certified Reference Material (CRM).

This instrument was calibrated under procedure No. **CLC-CPTH-04** [Temperature] based on **ASTM E 644-04** as calibration guidelines. The calibration was performed by using Calibration Bath, Precision Thermometer and IPRT which maintained by the Calibration Laboratory Co., Ltd.

REFERENCE STANDARD USED :

1. pH Standard Solution, NIMT TRM CODE TRM-S-2003, TRM CODE TRM-S-2007.
2. pH Standard Solution, Control Company Catalog Number 06664260,11754256, Lot Number CC787362.
3. Calibration Bath, Kambic Model OB-22/2 ULT S/N. 17115653.
4. Precision Thermometer, ASL Model F250 S/N. 1334023800.
5. IPRT, Wika Model CTP5000-250-D S/N. PO00043543-1-10-1.

Certificate No. **Q25070523**

F3-011-05/12-23

page 2 of 4



@clccalibration



CALIBRATION LABORATORY Co., LTD.

2/10-11,14, 55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



TRACEABILITY :

1. The measurements are traceable to International System of Units (SI) , through National Institute of Metrology (Thailand).
Lot Number. 080124 , 120124. Due Date 23 January 2026.
2. The measurements are traceable to International System of Units (SI) , through Control Company.
Certificate No. 4281-14495731 , Due Date 27 September 2025.
3. The measurements are traceable to International System of Units (SI) , through Calibration Laboratory Co., Ltd.
Certificate No. Q24120999, Due Date 26 November 2025.
4. The measurements are traceable to International System of Units (SI) , through Thailand Institute of Scientific and Technological Research (TISTR). Certificate No. PSL-T 1042/67, Due Date 16 October 2025.
5. The measurements are traceable to International System of Units (SI) , through National Institute of Metrology (Thailand).
Certificate No. TT-0146-24, Due Date 28 October 2025.

UNCERTAINTY :

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor complies with the table which for a normal distribution corresponds to a coverage probability of approximately 95 %.

It has been evaluated according to the "Evaluation of the Uncertainty of Measurement in Calibration (EA-4/02 M:2022)"

Certificate No. Q25070523

F3-011-05/12-23

page 3 of 4



@clccalibration




CLC
Accredited
ISO/IEC 17025

CALIBRATION LABORATORY Co., LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230

Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



CONDITION OF CALIBRATION ITEM : RECEIVED IN GOOD OPERATIONAL CONDITION

MEASUREMENT RESULTS : (X) without adjustment () adjustment

The table in the following gives the calibration results and associated measurement uncertainties of pH meter.

CALIBRATION DATA

1. pH METER RESULT @ 25 °C

Standard pH Buffer Solution (pH)	pH Meter Reading (pH)	pH Meter Reading (mV)	Correction (pH)	Uncertainty of pH Measurement ($\pm$ pH)	k Factor
4.003	4.005	168.2	-0.002	0.010	2,00
7.005	7.010	-8.1	-0.005	0.013	2,00
10.015	10.010	-177.7	+0.005	0.014	2,00

Technical Note. Setting function CAL 3 point (4,7,10).

Note. The Scope of Accredited ANAB Certificate No. ACDM-2814 Version 015 Page 4 of 68

2. TEMPERATURE RESULT

Immersion depth (mm)	Actual Temperature (°C)	DUC Reading (°C)	Correction (°C)	Uncertainty $\pm$ (°C)
100	25.00	25.0	0.00	0.07

Technical Note. Type of sensor : Thermistor

Probe $\varnothing$ 3 mm

Materials : Metal Sheath.

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor of $k = 2,00$.

Note. The Scope of Accredited ANAB Certificate No. ACDM-2814 Version 015 Page 56 of 68

This report is valid for the above stated instrument/s only.

End of Certificate

Certificate No. Q25070523

F3-011-05/12-23

page 4 of 4



@clccalibration

Certificate of Calibration

Certificate No. : 68-400046-2

Page : 1 of 2

Submitted by : S. P. S Consulting Service Co., Ltd.
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900

Equipment : Liquid in Glass Thermometer
 Manufacturer : SK Model : N/A
 Range : 0 °C to 100 °C Resolution : 1 °C
 Serial No. : N/A Immersion : Total
 ID No. : TM21/59

Environment : Ambient Temperature : (23 ± 2) °C
 Relative Humidity : (50 ± 15) %
 Line Voltage : (220 ± 22) VAC

Date of Received : 21 January 2025

Date of Calibration : 24 January 2025

Date of Issue : 24 January 2025

Calibrated by : Chortip Samchusri

Calibration Method : This instrument was calibrated by In-house method comparison technique CAL-M4001 based on ASTM E77-07 by compared with PRT in the liquid bath at the constant controlled temperature.

The temperature scale used was based on ITS-90

Reference Standard Instruments : This certification is traceable to the International System of Units

1. Platinum Resistance Thermometer (PRT)

ID No.	Cert. No.	Due Date	Traceability
400001	TT-0023-24	16 Feb 2026	National Institute of Metrology Thailand (NIMT)

2. Standard Digital Thermometer

ID No.	Cert. No.	Due Date	Traceability
400003	23E1866	01 Jun 2025	National Institute of Metrology Thailand (NIMT)
400004	23E1866	01 Jun 2025	National Institute of Metrology Thailand (NIMT)

Approved by :



(Permpoon Chanpu)

Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 68-400046-2

Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Function : Temperature measurement

Ice point check : UUC* reading 0 °C Standard reading 0.4429 °C

Standard Reading (°C)	UUC Reading (°C)	Correction (°C)	Uncertainty (± °C)
20.4801	20	0.5	0.31

Remark

UUC : Unit Under Calibration

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

- ๐0๐ -





CERTIFICATE No : 25M2256

REFERENCE No : 76365-3

PAGE : 1 OF 2

Certificate of Calibration

EQUIPMENT : DIGITAL BALANCE

MANUFACTURER : SARTORIUS

MODEL : BSA224S-CW

SERIAL No : 36591843


ID No : BA09/61

CONDITION AS RECEIVED : USED ITEM

SUBMITTED BY : S.P.S. CONSULTING SERVICE CO., LTD.
7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN RD.,
JOMPOL, CHATUCHAK, BANGKOK 10900

CALIBRATED BY : ATSAWIN Y.

CALIBRATION DATE : 07-Mar-25

APPROVED BY : 
PONGSAK J.

ISSUED DATE : 13-Mar-25

RECEIVED DATE : 07-Mar-25

THIS CERTIFICATE MAY NOT BE REPRODUCED OTHER THAN IN FULL EXCEPT WITH THE PRIOR WRITTEN APPROVAL OF
QUALITY CALIBRATION CO., LTD.





CERTIFICATE No : 25M2256

PAGE : 2 OF 2

Calibration Report

EQUIPMENT : DIGITAL BALANCE MODEL : BSA224S-CW
MANUFACTURER : SARTORIUS S/N : 36591843
ID No : BA09/61 RECEIVED DATE : 07-Mar-25
AIR PRESSURE : 1009mbar $\pm$ 1mbar CALIBRATION DATE : 07-Mar-25
AMBIENT TEMPERATURE : 24° C $\pm$ 1° C RELATIVE HUMIDITY : 52 %RH $\pm$ 10 % RH

CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED BY ACCORDING TO UKAS LAB 14 EDITION 6:2019 BY USING KNOWN WEIGHT STANDARD WEIGHT. THE BALANCE WAS NOT ADJUSTED BEFORE CALIBRATION. THE BALANCE HAS NO ZERO TRACKING FUNCTION. REPEATABILITY WAS MEASURED BY USING 10 REPEATED MEASUREMENTS. LINEARITY WAS MEASURED COVERING 10 POINTS, EVENLY SPREAD OVER THE RANGE. THE INSTRUMENT WAS SET ZERO BEFORE PERFORMING THE LINEARITY TEST. OFF-CENTER LOADING WAS MEASURED BY USING STANDARD WEIGHTS PLACED ON THE PAN AND MOVED TO VARIOUS POSITIONS ON THE PAN.

2. REFERENCE STANDARD INSTRUMENTS :-

<u>INSTRUMENT</u>	<u>MODEL</u>	<u>SERIAL No</u>	<u>CERTIFICATE No</u>	<u>DUE DATE</u>
1) STANDARD WEIGHT SET	E2	QK-I-151	C02250116	28-Jan-27
2) STANDARD WEIGHT	E2	15843	C02250117	29-Jan-27

3. THE CERTIFICATE IS VALID FOR THE ITEM CALIBRATED AS SHOWN ON THE DATE AND PLACE OF CALIBRATION ONLY.

4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.

5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-
- NATIONAL INSTITUTE OF METROLOGY (THAILAND)

RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

1. ZERO SETTING FUNCTION : NORMAL


2. TARE FUNCTION : NORMAL

3. REPEATABILITY OF READING AT 200 g WAS 0.000071 g

4. DEPARTURE FROM NOMINAL VALUE/ LINEARITY

NOMINAL VALUE (g)	BALANCE READING (g)	CORRECTION (g)	UNCERTAINTY ($\pm$ g)
0.00	0.0000	0.0000	0.00012
0.10	0.1000	0.0000	0.00012
0.20	0.2000	0.0000	0.00012
0.50	0.5000	0.0000	0.00012
1.00	1.0000	0.0000	0.00012
2.00	2.0000	0.0000	0.00012
5.00	5.0000	0.0000	0.00012
10.00	10.0000	0.0000	0.00012
20.00	20.0001	-0.0001	0.00012
50.00	50.0000	0.0000	0.00014
100.00	100.0001	-0.0001	0.00019
200.00	200.0001	-0.0001	0.00032

5. OFF CENTER LOADING ERROR



POINT	READING (g)
1	100.0000
2	100.0000
3	100.0000
4	100.0000
5	100.0000
OFF-CENTER LOADING	0.0000

NOTE: THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA
THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR $k=2$, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT



CERT.No.: HS-W015C

Calibration Date : 18 Mar 25
 Submitted by : S.P.S CONSULTING SERVICE CO.,LTD
 7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol,
 Chatuchak, Bangkok, Thailand 10900

Avg Room Temp : 20 °C
 Avg Water Temp : 20 °C
 Air Pressure : 760.00 mmHg
 Salinity : 0 ppt

Model : YSI 5000
 S/N : 15B100751
 Probe : YSI 5010
 S/N : 22D100097
 ID NO. : -
 Air Temp ref : S/N. F8065C26
 Barometric ref : S/N. F8065C26
 Water Temp ref : -
 ID NO. HS001
 Technician : Kittipong M.

Calibration Details

Calibration Point	100% air sat. (@20 °C, DO = 9.09 mg/l)	(status)	(status)
Measurement 1 (mg/l)	9.08	(PASS)	-
Measurement 2 (mg/l)	9.08	(PASS)	-
Measurement 3 (mg/l)	9.08	(PASS)	-
Measurement 4 (mg/l)	9.07	(PASS)	-
Measurement 5 (mg/l)	9.07	(PASS)	-
Measurement 6 (mg/l)	9.07	(PASS)	-
Measurement 7 (mg/l)	9.07	(PASS)	-
Measurement 8 (mg/l)	9.07	(PASS)	-
Measurement 9 (mg/l)	9.07	(PASS)	-
Measurement 10 (mg/l)	9.07	(PASS)	-

Mean Measurement	9.07	mg/l	-	-
Inaccuracy	0.02	mg/l	-	-

Overall Status (PASS)

Manufacturer Specification

Accuracy = +/- 0.02 mg/l

- 1) This certificate is issued based on the result that are found as shown on date and place of test only.
- 2) The calibration procedure followed in accordance with Harikul Science Co., Ltd.
- 3) This result shall not be used for advertising purpose.



Technician Signature
 (Kittipong Maekwong)



Laboratory Manager
 (Natenapha Pisatkunchon)



QUALITY CALIBRATION CO., LTD.

235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160

Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

www.qcalibration.com

CERTIFICATE No : 25T0520

REFERENCE No : 75853-1

PAGE : 1 OF 2

Certificate of Calibration

EQUIPMENT : COD REACTOR

MANUFACTURER : HACH

MODEL : DRB 200

SERIAL No : 15110C0497


ID No : DRB 05/59

CONDITION AS RECEIVED : USED ITEM

SUBMITTED BY : S.P.S. CONSULTING SERVICE CO., LTD.
7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN RD.,
JOMPOL, CHATUCHAK, BANGKOK 10900

CALIBRATED BY : CHAICHARN CH.

CALIBRATION DATE : 27-Jan-25

APPROVED BY : 
PONGSAK J.

ISSUED DATE : 27-Jan-25

RECEIVED DATE : 15-Jan-25

THIS CERTIFICATE MAY NOT BE REPRODUCED OTHER THAN IN FULL EXCEPT WITH THE PRIOR WRITTEN APPROVAL OF
QUALITY CALIBRATION CO., LTD.



F-G010 REV : 03



QUALITY CALIBRATION CO., LTD.

235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160

Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

CERTIFICATE No : 25T0520

PAGE : 2 OF 2

Calibration Report


EQUIPMENT : COD REACTOR
MANUFACTURER : HACH
ID NUMBER : DRB 05/59
RECEIVED DATE : 15-Jan-25
AMBIENT TEMPERATURE : 23° C ± 1° C
MODEL : DRB 200
SERIAL NUMBER : 15110C0497
CALIBRATION DATE : 27-Jan-25
RELATIVE HUMIDITY : 53 %RH ± 10 % RH

CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED BY DIRECT MEASUREMENT METHOD WITH CALIBRATED THERMOCOUPLE TYPE K UNDER NO LOAD CONDITION. THE THERMOCOUPLES WERE PLACED ON POINTS AND LOCATED AS THE PICTURE.
2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) DATA LOGGER WITH TC TYPE K	HYDRA 2635A	6635300	24T6468	26-Jun-25
3. THE CERTIFICATE IS VALID FOR THE ITEM CALIBRATED AS SHOWN ON THE DATE AND PLACE OF CALIBRATION ONLY.
4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.
5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-
- NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH QUALITY CALIBRATION CO., LTD.

RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

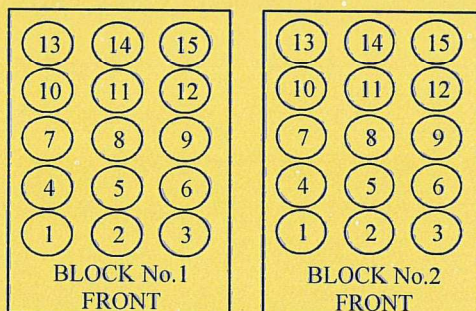

Block No.	1	2
Calibration Point (°C)	150	150
Controller temperature (°C)	144	144
Indicating Temperature	144	144
Measured Temperature (°C) at Spread Locations	1	150.01
	2	150.69
	3	150.40
	4	150.22
	5	150.27
	6	150.51
	7	150.24
	8	150.20
	9	150.14
	10	149.70
	11	149.58
	12	149.46
	13	148.77
	14	148.99
	15	149.02
Uncertainty of Measurement(± °C)	0.87	0.87

NOTE 1 : THE UNCERTAINTY OF MEASUREMENT EXCLUDED TEMPERATURE UNIFORMITY OF THE CHAMBER.

NOTE 2 : LOCATION 10 WAS REFERENCE LOCATION.

NOTE 3 : THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA.

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR $k=2$, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT



GC Clarus 600/680 Preventive Maintenance (PM)

Company Name:	S.P.S. Consulting Service Co.,Ltd		
Address (Instrument Location):	7 Soi Phaholyothin24 Phaholyothin Road, Jompol, Chatuchak, Bangkok, 10900.		
Serial Number:	680S14042502	Service Tag:	N68APSSFEMP
Customer Name (if applicable):	Ms.Naruecha	PM number:	1 of 2
Service Engineer Name:	Monchai Kitcharoenkeat	Service Order Number:	WO-
Date PM Performed: (DD-MMM-YYYY)	22-Feb-2025	Next PM Due Date: (DD-MMM-YYYY)	22-Aug-2025

Part Number	Release	Publication Date	
TH09370070	C	August 2016	

Scope

The purpose of this PM is to ensure the continued functionality of the Clarus 600 and Clarus 680 GC by inspecting and replacing any worn or damaged parts. This service should only be performed by a trained representative of PerkinElmer. The customer should save their method before the PM begins.

General Instructions:

The customer must provide the engineer operational data to demonstrate recent instrument performance prior to starting the PM. Always check with the customer before making any changes that may affect the customer's analysis or calibration, including a current back-up of system software and/or data files. The completed document should be signed by an authorized PerkinElmer and customer representative and left with the customer. Update the PM sticker and instrument logbook as required.

Copyright Information

This document contains proprietary information that is protected by copyright. All rights are reserved. No part of this publication may be reproduced in any form whatsoever or translated into any language without the prior, written permission of Perkin Elmer, Inc. **Copyright © 2013 PerkinElmer, Inc.**

Trademarks

Registered names, trademarks, etc. used in this document, even when not specifically marked as such, are protected by law. PerkinElmer is a registered trademark of PerkinElmer, Inc. All other trademarks and registered trademarks not owned by PerkinElmer, Inc. or its subsidiaries that are depicted herein are the property of their respective owners. **Except as specifically set forth in its terms and conditions of sale, PerkinElmer makes no Warranty of any kind with regard to this document, including, but not limited to, the implied warranties of merchantability and fitness for a particular purpose.** PerkinElmer shall not be liable for incidental or consequential damages in connection with the furnishing or use of this document.

Component List

Component / Specific Model	Serial #	Software Version	Configuration Notes
Clarus680	680S14042502	Totalchrom6.3.2	PSS, PSS, FID,
Clarus SQ8T	648N4050804	Turbomass 6.4	
AtomX	US14113002	Tekma AtomX	

Parts Lists

Additional Tools Required for PM				
Part Number (if applicable)	Description	Quantity	Serial #	Calibration Due Date (MM/YY)
N/A				
Additional Reagents and Standards Required for PM				
Part Number (if applicable)	Description	Quantity	Batch/Lot #	Expiration Date (MM/YY)
N/A				

Procedure Checklist

Use (✓) to check off those steps in the checklist that have been completed.

1. General:

- ☒ Review the instrument performance with the customer and document any recent problems.

- ☒ Check incoming AC line voltage for proper levels and grounding.

L-N 220 Volt

L-G 220 Volt

N-G 0.33 Volt

**Neutral to ground not more than 0.5 volts peak to peak*

- ☒ Inspect all gas line filters and traps; Replace if necessary with customer supplied spares.

Carrier gas ☒ Helium ☐ Nitrogen ☐ Hydrogen

Moisture level ☒ Good ☐ Need to replace ☐ Other _____

Detector gas ☒ Air Zero ☒ Hydrogen ☐ Nitrogen ☐ Helium

Moisture level ☒ Good ☐ Need to replace ☐ Other _____

- ☒ Inspect the customer log book and make any appropriate PM entries.

- ☒ Leak check all fittings from the gas source to instrument.

Gas leakage ☒ Pass ☐ Fail Comment _____

- ☒ Perform general inspection of system for cleanliness.

- ☒ Inspect for functional and clean electronic cooling and oven vent fans

Electronic cooling fan ☒ Yes ☐ No

Oven cooling fan ☒ Yes ☐ No

2. Electronic :

- ☒ Check oven temperature. Calibrate if necessary.

Oven temperature set point 150 °C ☒ Pass ☐ Fail

- ☐ Check sub-ambient option. (If installed).

Oven temperature set point 5 °C ☐ Pass ☐ Fail

- ☒ Perform routine maintenance on detector/injector. Replace parts as necessary with customer supplied spares.

- ☒ Check flows, including split flows if applicable. Calibrate if necessary.

Carrier flow	Pass
Split flow	Pass
- ☒ Check detector gas flows and adjust if necessary.

Detector flow	Pass
---------------	------
- ☒ Autosampler installed ☒ Yes ☐ No

Check autosampler sensor for wear and replace if necessary.	
Vial sensor	Pass
Door sensor	Pass
Tower sensor	Pass
Plunger sensor	Pass
Elevator sensor	Pass
- ☒ Remove syringe, manually flush. Replace with customer supplied spare if necessary.
- ☒ Check firmware version. Upgrade to current levels if necessary.

Firmware version	<u>6.5</u>
------------------	------------
- ☒ Measure all accessible power supply voltages.

5 Volt	Pass
+15 Volt	Pass
-15 Volt	Pass
24 Volt	Pass
- ☒ Record all detector voltage signal.

Detector Channel A	<u>1.12</u>	mV.
Detector Channel B	<u>NA</u>	mV.

3. Diagnostics Tests:

- ☒ Run instrument diagnostics.

☒ BRAM	Pass
☒ EPROM	Pass
- ☒ Run Autosampler diagnostics.

☒ BRAM	Pass
☒ EPROM	Pass

4. Review:

- ☒ Review with the customer PM work performed.
- ☒ Review with the customer routine maintenance procedures.
- ☒ Discuss recommended customer-supplied materials to have on hand
- ☒ Attach PM sticker.
- ☒ Update Logbook.

Additional Comments

Additional Comments Regarding the PM

Review

<i>The preventive maintenance checks and if applicable performance tests for Clarus600/680 GC have been completed.</i>		
<i>This Clarus600/680 GC Pass the preventive maintenance.</i>		
Review of Preventive Maintenance:		
Authorized PerkinElmer Representative: Monchai Kitcharoenkeat	<i>Monchai</i>	Date: 22-Feb-2025 (DD-MMM-YYYY)
Authorized Customer Representative: Ms.Naruecha	<i>Naruecha</i>	Date: 22-Feb-2025 (DD-MMM-YYYY)

GC Clarus 600/680 Preventive Maintenance (PM)

Company Name:	S.P.S. Consulting Service Co.,Ltd		
Address (Instrument Location):	7 Soi Phaholyothin24 Phaholyothin Road, Jompol, Chatuchak, Bangkok, 10900.		
Serial Number:	680S14042502	Service Tag:	N68APSSFEMP
Customer Name (if applicable):	Ms.Naruecha	PM number:	2 of 2
Service Engineer Name:	Monchai Kitcharoenkeat	Service Order Number:	WO-06815714
Date PM Performed: (DD-MMM-YYYY)	13-Aug-2025	Next PM Due Date: (DD-MMM-YYYY)	13-Feb-2026

Part Number	Release	Publication Date	
TH09370070	C	August 2016	

Scope

The purpose of this PM is to ensure the continued functionality of the Clarus 600 and Clarus 680 GC by inspecting and replacing any worn or damaged parts. This service should only be performed by a trained representative of PerkinElmer. The customer should save their method before the PM begins.

General Instructions:

The customer must provide the engineer operational data to demonstrate recent instrument performance prior to starting the PM. Always check with the customer before making any changes that may affect the customer's analysis or calibration, including a current back-up of system software and/or data files. The completed document should be signed by an authorized PerkinElmer and customer representative and left with the customer. Update the PM sticker and instrument logbook as required.

Copyright Information

This document contains proprietary information that is protected by copyright. All rights are reserved. No part of this publication may be reproduced in any form whatsoever or translated into any language without the prior, written permission of Perkin Elmer, Inc. **Copyright © 2013 PerkinElmer, Inc.**

Trademarks

Registered names, trademarks, etc. used in this document, even when not specifically marked as such, are protected by law. PerkinElmer is a registered trademark of PerkinElmer, Inc. All other trademarks and registered trademarks not owned by PerkinElmer, Inc. or its subsidiaries that are depicted herein are the property of their respective owners. **Except as specifically set forth in its terms and conditions of sale, PerkinElmer makes no Warranty of any kind with regard to this document, including, but not limited to, the implied warranties of merchantability and fitness for a particular purpose.** PerkinElmer shall not be liable for incidental or consequential damages in connection with the furnishing or use of this document.

Component List

Component / Specific Model	Serial #	Software Version	Configuration Notes
Clarus680	680S14042502	Totalchrom6.3.2	PSS, PSS, FID,
Clarus SQ8T	648N4050804	Turbomass 6.4	
AtomX	US14113002	Tekma AtomX	

Parts Lists

Additional Tools Required for PM				
Part Number (if applicable)	Description	Quantity	Serial #	Calibration Due Date (MM/YY)
N/A				
Additional Reagents and Standards Required for PM				
Part Number (if applicable)	Description	Quantity	Batch/Lot #	Expiration Date (MM/YY)
N/A				

Procedure Checklist

Use (✓) to check off those steps in the checklist that have been completed.

1. General:

- ☒ Review the instrument performance with the customer and document any recent problems.

- ☒ Check incoming AC line voltage for proper levels and grounding.

L-N 220 Volt

L-G 220 Volt

N-G 0.32 Volt

**Neutral to ground not more than 0.5 volts peak to peak*

- ☒ Inspect all gas line filters and traps; Replace if necessary with customer supplied spares.

Carrier gas ☒ Helium ☐ Nitrogen ☐ Hydrogen

Moisture level ☒ Good ☐ Need to replace ☐ Other _____

Detector gas ☒ Air Zero ☒ Hydrogen ☐ Nitrogen ☐ Helium

Moisture level ☒ Good ☐ Need to replace ☐ Other _____

- ☒ Inspect the customer log book and make any appropriate PM entries.

- ☒ Leak check all fittings from the gas source to instrument.

Gas leakage ☒ Pass ☐ Fail Comment _____

- ☒ Perform general inspection of system for cleanliness.

- ☒ Inspect for functional and clean electronic cooling and oven vent fans

Electronic cooling fan ☒ Yes ☐ No

Oven cooling fan ☒ Yes ☐ No

2. Electronic :

- ☒ Check oven temperature. Calibrate if necessary.

Oven temperature set point 150 °C ☒ Pass ☐ Fail

- ☐ Check sub-ambient option. (If installed).

Oven temperature set point 5 °C ☐ Pass ☐ Fail

- ☒ Perform routine maintenance on detector/injector. Replace parts as necessary with customer supplied spares.

- ☒ Check flows, including split flows if applicable. Calibrate if necessary.

Carrier flow	Pass
Split flow	Pass
- ☒ Check detector gas flows and adjust if necessary.

Detector flow	Pass
---------------	------
- ☒ Autosampler installed ☒ Yes ☐ No

Check autosampler sensor for wear and replace if necessary.	
Vial sensor	Pass
Door sensor	Pass
Tower sensor	Pass
Plunger sensor	Pass
Elevator sensor	Pass
- ☒ Remove syringe, manually flush. Replace with customer supplied spare if necessary.
- ☒ Check firmware version. Upgrade to current levels if necessary.

Firmware version	<u>6.5</u>
------------------	------------
- ☒ Measure all accessible power supply voltages.

5 Volt	Pass
+15 Volt	Pass
-15 Volt	Pass
24 Volt	Pass
- ☒ Record all detector voltage signal.

Detector Channel A	<u>0.98</u>	mV.
Detector Channel B	<u>NA</u>	mV.

3. Diagnostics Tests:

- ☒ Run instrument diagnostics.

☒ BRAM	Pass
☒ EPROM	Pass
- ☒ Run Autosampler diagnostics.

☒ BRAM	Pass
☒ EPROM	Pass

4. Review:

- ☒ Review with the customer PM work performed.
- ☒ Review with the customer routine maintenance procedures.
- ☒ Discuss recommended customer-supplied materials to have on hand
- ☒ Attach PM sticker.
- ☒ Update Logbook.

Additional Comments

Additional Comments Regarding the PM

Review

<i>The preventive maintenance checks and if applicable performance tests for Clarus600/680 GC have been completed.</i>	
<i>This Clarus600/680 GC Pass the preventive maintenance.</i>	
Review of Preventive Maintenance:	
Authorized PerkinElmer Representative: Monchai Kitcharoenkeat <i>Monchai</i>	Date: 13-Aug-2025 (DD-MMM-YYYY)
Authorized Customer Representative: Ms.Naruecha <i>Naruecha</i>	Date: 13-Aug-2025 (DD-MMM-YYYY)

ระดับเสียงในชุมชน



THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-68/0220

MTC No. EEL. BP. 44/0268

CALIBRATION CERTIFICATE

Submitted by : S.P.S.Consulting Service Co.,Ltd.

Address : 7 Soi Phaholyothin 24, Phaholyothin Road, Jompol, Chatuchak, Bangkok 10900.

Calibrated at : Electrical and Electronic Standards Laboratory, Industrial Metrology and Testing Service Centre.
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Rd., Muang, Samutprakan 10280.

Instrument Calibrated :

Description : Sound Calibrator

Manufacturer : ACO

Model : 2127

Serial No. : 130006

Ambient Environment

Temperature : $(23 \pm 3) ^\circ\text{C}$

Relative Humidity : $(50 \pm 15) \%$

Ambient Pressure : $(101.325 \pm 1.500) \text{ kPa}$

- Standards used :
1. Digital Function Synthesizer NF Electronic DF-193A S/N 122037.
 2. Measuring Amplifier Bruel&Kjaer 2636 S/N 1537484.
 3. Programmable Attenuator Tamagawa TPA-303A S/N OF 2214.
 4. Digital Multimeter Agilent 34401A S/N MY44005560.
 5. Pressure Transmitter Vaisala PTB202AD S/N T0650001.
 6. Audio Analyzer Panasonic VP-7722A S/N 041477D122.
 7. Condenser Microphone B&K 4180 S/N 2889871.

Calibration Procedure: CP-102-04 based on IEC 60942-2003; The sound pressure level generated by sound calibrator under test shall be measured by standard microphone using an insert voltage technique.

This instrument has been calibrated against standards maintained at Electrical and Electronic Standards Laboratory (EEL), which are traceable to the International System of Units through the National Institute of Metrology (Thailand).

The information on actual reading is attached herewith and the uncertainty limits quoted refer to the measured values only.

Date of Receipt : 19 Feb. 2025

Date of Calibration : 21 Feb. 2025

1 / 2
W

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.5

Head Office

35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9009

Office/Laboratory

668 Mu 2 Tambon Bangpoomai, Amphoe Muang Samutprakan,
Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtc@tistr.or.th Website : www.tistr.or.th

Office

196 Phahonyothin Road, Ladyao, Chatuchak,
Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827

THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-68/0220

MTC No. EEL. BP. 44/0268

The reported expanded uncertainty is based upon a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%.

Nominal Output of Unit Under Test = 94 dB re 20 μ Pa at 1000 Hz

Acoustic Output in dB re 20 μ Pa, Corrected to Reference Conditions: 101.325 kPa, 23.0 °C and 50 %RH.

1. Sound Pressure Level

Standard Microphone Type	Measured Sound Pressure Level (dB)	Deviated value (dB)	Uncertainty (dB)	Tolerance limit IEC60942:2003 Class 1
1/2 inch Bruel&Kjaer 4180	93.81	-0.19	± 0.10	± 0.40 dB

2. Frequency

Standard Microphone Type	Measured Frequency (Hz)	Deviated value (Hz)	Uncertainty (Hz)	Tolerance limit IEC60942:2003 Class 1
1/2 inch Bruel&Kjaer 4180	999.9	-0.1	± 1.5	$\pm 1.0\%$

3. Total Distortion


Standard Microphone Type	Measured Total Distortion (%)	Uncertainty (%)	Tolerance limit IEC60942:2003 Class 1
1/2 inch Bruel&Kjaer 4180	0.95	± 0.50	$\pm 3.0\%$

Note : 1. No adjustment.

2. The calibrator pressure correction was not included.

3. The microphone volume correction was not included.

Calibrated by :


(Mr. Weerachai Deechaiyae)

Approved by :


(Mr. Prawate Kluaypa)
Director

Date of Calibration : 21 Feb. 2025

Date of Issue : 24 Feb. 2025

Electrical and Electronic Standards Laboratory
Industrial Metrology and Testing Service Centre

Ref : 2011268021900739001

End of Certificate

2 / 2

The results relate only to the items tested/calibrated or value assigned.
Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.5

Head Office

35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9009

Office/Laboratory

668 Mu 2 Tambon Bangpoornai, Amphoe Muang Samutprakan,
Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtc@tistr.or.th Website : www.tistr.or.th

Office

196 Phahonyothin Road, Ladyao, Chatuchak,
Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72. Fax : (662) 513-4221. E-mail : sale@spscon.com., www.spscon.com

Noise R_719/25

Sound Level Meter Calibration Report

Acoustic Calibrator Data

Brand	ACO	Number	AC 03/56
Model	2127	Serial No.	130006
Calibration Range	94 dB, 1000 Hz	Last Calibration	21 February 2025
		Due Date	21 February 2026

Calibration Data

Sound Level Meter Data				Calibration Data		
SLM No.	Brand	Model	Serial No.	Date	Actual Reading [dB]	
					Before Adjustment	After Adjustment
ACO-R12	ACO	6236	00172040	03 December 2025	93.9	93.9
ACO-R28	ACO	6236	00192040	03 December 2025	93.9	93.9
Acoustic Certified Value : Thailand Institute of Scientific and Technological Research (TISTR)					93.81 ± 0.10 dB	

Calibrated by :

Adul Dangklom
(Mr. Adul Dangklom)

Approved by :

Peera Detudom
(Mr. Peera Detudom)

ระดับเสียงเฉลี่ยตลอดระยะเวลาการทำงาน



THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-68/0220

MTC No. EEL. BP. 44/0268

CALIBRATION CERTIFICATE

Submitted by : S.P.S.Consulting Service Co.,Ltd.

Address : 7 Soi Phaholyothin 24, Phaholyothin Road, Jompol, Chatuchak, Bangkok 10900.

Calibrated at : Electrical and Electronic Standards Laboratory, Industrial Metrology and Testing Service Centre.
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Rd., Muang, Samutprakan 10280.

Instrument Calibrated :

Description : Sound Calibrator

Manufacturer : ACO

Model : 2127

Serial No. : 130006

Ambient Environment

Temperature : $(23 \pm 3) ^\circ\text{C}$

Relative Humidity : $(50 \pm 15) \%$

Ambient Pressure : $(101.325 \pm 1.500) \text{ kPa}$

- Standards used :**
1. Digital Function Synthesizer NF Electronic DF-193A S/N 122037.
 2. Measuring Amplifier Bruel&Kjaer 2636 S/N 1537484.
 3. Programmable Attenuator Tamagawa TPA-303A S/N OF 2214.
 4. Digital Multimeter Agilent 34401A S/N MY44005560.
 5. Pressure Transmitter Vaisala PTB202AD S/N T0650001.
 6. Audio Analyzer Panasonic VP-7722A S/N 041477D122.
 7. Condenser Microphone B&K 4180 S/N 2889871.

Calibration Procedure: CP-102-04 based on IEC 60942-2003; The sound pressure level generated by sound calibrator under test shall be measured by standard microphone using an insert voltage technique.

This instrument has been calibrated against standards maintained at Electrical and Electronic Standards Laboratory (EEL), which are traceable to the International System of Units through the National Institute of Metrology (Thailand).

The information on actual reading is attached herewith and the uncertainty limits quoted refer to the measured values only.

Date of Receipt : 19 Feb. 2025

Date of Calibration : 21 Feb. 2025

1 / 2
W

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.5

Head Office

35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9009

Office/Laboratory

668 Mu 2 Tambon Bangpoomai, Amphoe Muang Samutprakan,
Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtc@tistr.or.th Website : www.tistr.or.th

Office

196 Phahonyothin Road, Ladyao, Chatuchak,
Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827

THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-68/0220

MTC No. EEL. BP. 44/0268

The reported expanded uncertainty is based upon a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%.

Nominal Output of Unit Under Test = 94 dB re 20 μ Pa at 1000 Hz

Acoustic Output in dB re 20 μ Pa, Corrected to Reference Conditions: 101.325 kPa, 23.0 °C and 50 %RH.

1. Sound Pressure Level

Standard Microphone Type	Measured Sound Pressure Level (dB)	Deviated value (dB)	Uncertainty (dB)	Tolerance limit IEC60942:2003 Class 1
1/2 inch Bruel&Kjaer 4180	93.81	-0.19	± 0.10	± 0.40 dB

2. Frequency

Standard Microphone Type	Measured Frequency (Hz)	Deviated value (Hz)	Uncertainty (Hz)	Tolerance limit IEC60942:2003 Class 1
1/2 inch Bruel&Kjaer 4180	999.9	-0.1	± 1.5	$\pm 1.0\%$

3. Total Distortion

Standard Microphone Type	Measured Total Distortion (%)	Uncertainty (%)	Tolerance limit IEC60942:2003 Class 1
1/2 inch Bruel&Kjaer 4180	0.95	± 0.50	$\pm 3.0\%$

Note : 1. No adjustment.

2. The calibrator pressure correction was not included.

3. The microphone volume correction was not included.

Calibrated by :


(Mr. Weerachai Deechaiyae)

Approved by :


(Mr. Prawate Kluaypa)
Director

Date of Calibration : 21 Feb. 2025

Date of Issue : 24 Feb. 2025

Electrical and Electronic Standards Laboratory
Industrial Metrology and Testing Service Centre

Ref : 2011268021900739001

End of Certificate

2 / 2

The results relate only to the items tested/calibrated or value assigned.
Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.5

Head Office

35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9009

Office/Laboratory

668 Mu 2 Tambon Bangpoornai, Amphoe Muang Samutprakan,
Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtc@tistr.or.th Website : www.tistr.or.th

Office

196 Phahonyothin Road, Ladyao, Chatuchak,
Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

Noise R_627/25

Sound Level Meter Calibration Report

Acoustic Calibrator Data

Brand	ACO	Number	AC 03/56
Model	2127	Serial No.	130006
Calibration Range	94 dB, 1000 Hz	Last Calibration	21 February 2025
		Due Date	21 February 2026

Calibration Data

Sound Level Meter Data				Calibration Data		
SLM No.	Brand	Model	Serial No.	Date	Actual Reading [dB]	
					Before Adjustment	After Adjustment
ACO-B29	ACO	6236	00182011	09 November 2025	93.9	93.9
ACO-R40	ACO	6236	00192052	09 November 2025	93.9	93.9
ACO-R41	ACO	6236	00192053	09 November 2025	93.9	93.9
Acoustic Certified Value : Thailand Institute of Scientific and Technological Research (TISTR)					93.81 ± 0.10 dB	

Calibrated by :

Adul Dangklom
(Mr. Adul Dangklom)

Approved by :

Peera Detudom
(Mr. Peera Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72. Fax : (662) 513-4221. E-mail : sale@spscon.com, www.spscon.com

Noise R_624/25

Sound Level Meter Calibration Report

Acoustic Calibrator Data

Brand	ACO	Number	AC 03/56
Model	2127	Serial No.	130006
Calibration Range	94 dB, 1000 Hz	Last Calibration	21 February 2025
		Due Date	21 February 2026

Calibration Data

Sound Level Meter Data				Calibration Data		
SLM No.	Brand	Model	Serial No.	Date	Actual Reading [dB]	
					Before Adjustment	After Adjustment
ACO-R40	ACO	6236	00192052	09 November 2025	93.9	93.9
Acoustic Certified Value : Thailand Institute of Scientific and Technological Research (TISTR)					93.81 ± 0.10 dB	

Calibrated by :

Adul Dangklom
(Mr. Adul Dangklom)

Approved by :

Peera Detudom
(Mr. Peera Detudom)