

## ภาคผนวก จ

เอกสารสอบเทียบเครื่องมือตรวจวัด

## List of Instrument Certificates for Environmental Quality Analysis

No.	Instrument/Equipment	Parameter	Manufacturer	Model/Serial No.	Calibrator	Certification No.	Date of Calibration	Due date of Calibration*
1	Analytical Balance	FAT OIL AND GREASE	Mettler Toledo	AB204-S/FACT / 1129361010	United Analyst and Engineering Consultant Co., Ltd.	250422 1 BL002 25	23/4/2025	22/4/2026
2	Analytical Balance	TOTAL DISSOLVED SOLIDS	Mettler Toledo	XSR205DU / C210685394	National Food Institute,Ministry of Industry, Thailand	2502226-002-01	20/3/2025	19/3/2026
3	Analytical Balance	TOTAL SUSPENDED SOLIDS	Mettler Toledo	XSR205DU / C009071872	National Food Institute,Ministry of Industry, Thailand	2502226-001-01	20/3/2025	19/3/2026
4	Auto Clave	TOTAL COLIFORM BACTERIA	ALP Co.,Ltd. (Japan)	CL-40L / 810010	National Food Institute Ministry of Industry (Thailand)	2503287-001-01	5/6/2025	4/6/2026
5	BOD Incubator	BIOCHEMICAL OXYGEN DEMAND	ARCO	UR-1320 / -	Technology Promotion Association (Thailand-Japan)	25TM577	19/3/2025	19/3/2026
6	DO Meter	BIOCHEMICAL OXYGEN DEMAND	YSI	5100 / 11B 101863	Technology Promotion Association (Thailand-Japan)	25TW29	17/2/2025	16/2/2026
7	Digestion Units	TOTAL KJELDAHL NITROGEN	Foss Tecator	2520 Auto / 91794469	National Food Institute Ministry of Industry, Thailand	2501440-001-01	27/1/2025	26/1/2026
8	Incubator	TOTAL COLIFORM BACTERIA	Binder	KB400 / 20220000022479	National food institute ministry of Industry	2503682 004 01	1/7/2025	30/6/2026
9	Incubator	FECAL COLIFORM BACTERIA	Memmert	IPP260 / V616.0066	National Food Institute, Ministry of Industry, Thailand	2502229-002-01	19/3/2025	18/3/2026
10	Kjeltec System Distilling Unit	TOTAL KJELDAHL NITROGEN	Foss Tecator (Labtec)	KT200 / 91790524	FOSS South East Asia	13319	27/1/2025	26/1/2026
11	pH Meter	pH	YSI Environmental	pH 100A / JC02729	Technology Promotion Association (Thailand-Japan)	25CH861	23/7/2025	22/7/2026
12	Water Bath	FECAL COLIFORM BACTERIA	Memmert	WNE 14 / L414.1407	Technology Promotion Association (Thailand-Japan)	25TM501	19/3/2025	18/3/2026

**Due Date of Calibration\*** : Based on the annual calibration plan. At least 1 time per year.

# เอกสารไม่ควบคุม

Certificate No.: 250422-1-BL002-25

Code No.: BL002-25

Page: 2 of 3

Equipment: Electronic Balance

Manufacturer: Mettler Toledo

Model: AB204-S/FACT

Readability: 0.0001 g

Serial No.: 1129361010

ID No.: UAE.WAS.002/2552

Max. Capacity: 220 g

Calibration Date: April 23, 2025

Condition As-Received: In Condition

Condition of Equipment:

Condition of This Result of Calibration:

1. Calibration Method: This instrument was calibrated by method UAE.CP.CAL.006 In-House Method based on UKAS Lab 14 : 2022

2. Reference Standards:

Reference Standard:	Model	Serial No.	Calibrated By	Certificate No.	Traceability	Due Date
Standard Weight Class E2 (OIML)	1 mg to 1 kg	8749109122	AMARC	25-009359	Mettler-Toledo	21-Jan-27
Standard Weight Class F1 (OIML)	1 mg to 200 g	11119512	AMARC	24-013840	Mettler-Toledo	04-Feb-26
Instrument	Model	Serial No.	Calibrated By	Certificate No.	Traceability	Due Date
Thermo-Hygro-Baro Meter	MHB-3825D	AK.46457	SUCCESS	5G-H-00997/67	Success Gateway	21-Nov-25
Thermo-Hygro-Baro Meter	MHB-3825D	AK.46457	TPA	25P795	TPA	25-Feb-26

3. This certification is traceable to SI Unit

4. This certification was certified only for the instrument we calibrated

5. This result of calibration was found accurate as shown on date and place of calibration only.

6. Through the reference standard laboratory of AMARC 25-009359 Calibration 0152

Calibration Result:




1. Repeatability of Reading:

Nominal Value (g)	Standard Deviation of Reading (g)
200*	0.000045

2. Eccentric or off-center loading

A mass of 100 g was placed and moved to various positions on the pan

The Balance reading obtained is given in the table.



1 (g)	2 (g)	3 (g)	4 (g)	5 (g)	Maximum Difference (g)
100.0000	99.9996	99.9997	100.0003	100.0005	0.0005

เอกสารไม่ควบคุม

Certificate No.: 250422-1-BL002-25

Code No.: BL002-25

Page: 3 of 3

Equipment: Electronic Balance

Manufacturer: Mettler Toledo

Model: AB204-S/FACT

Readability: 0.0001 g

Serial No.: 1129361010

ID No.: UAE.WAS.002/2552

Max. Capacity: 220 g

Calibration Date: April 23, 2025

Calibration Result: (Continued)

Calibration Range: 0 - 200 g

Calibration Adjustment: Internal Calibration

3. Error of Indication from nominal or conventional mass value:

Nominal Value (g)	Reference Value (g)	Indication (g)	Correction (g)	Uncertainty ( $\pm$ mg)	Coverage Factor <i>k</i>
Unload	0.0000000	0.0000	0.0000	0.10	2.05
0.01	0.0100025	0.0099	0.0001	0.10	2.05
0.05	0.0500056	0.0500	0.0000	0.10	2.05
0.1	0.1000012	0.0999	0.0001	0.10	2.05
0.5	0.5000133	0.5000	0.0000	0.10	2.05
1	1.0000105	1.0000	0.0000	0.10	2.05
10	10.000010	10.0000	0.0000	0.11	2.04
40	40.000076	40.0000	0.0000	0.14	2.00
50	50.000056	50.0000	0.0001	0.13	2.00
80	80.000107	80.0000	0.0001	0.18	2.00
100	100.000109	99.9999	0.0002	0.17	2.00
120	120.00015	119.9999	0.0003	0.21	2.00
150	150.000165	149.9998	0.0003	0.24	2.00
160	160.000175	159.9997	0.0005	0.26	2.00
200	200.000129	199.9998	0.0004	0.30	2.00

4. Effect of Tare test:

Tare Load (g)	Test Load (g)	Indication (g)	Correction (g)
100	20.000041	19.9999	0.0001
	40.000076	39.9998	0.0002
	60.000066	59.9997	0.0003
	80.000107	79.9999	0.0002
	100.000168	100.0004	-0.0003

Remark:

The report uncertainty of measurement was based on standard uncertainty multiplied by coverage factor *k*, providing a level of confidence of approximately 95%.

เอกสารไม่ควบคุม





## Calibration Report

**Certificate No.:** 2502226-002-01

**Equipment:**

Electronic Balance

**Manufacturer:** METTLER TOLEDO

**Model:** XSR205DU

**Resolution:** 0.00001 g / 0.0001 g

**Serial No.:** C210685394

**ID No.:** UAE.WAO.010/2565

**Capacity:** 82 g / 220 g

**Date of Calibration:** 20 March 2025

Page 2 of 4

**Environment Condition:** Ambient Temperature:  $21.2 \pm 0.6$  °C Relative Humidity:  $48 \pm 3.5$  %

**Place of Calibration:** 208 Balance Room, UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.

**Condition of Equipment:** Good Condition

**Condition of This Results of Calibration:**

1. Calibration Method: NFI Method W-MA-001 In-House Method based on UKAS Lab 14 : 2019

2. Reference Standards:

Reference Standard	Model	Serial No.	Calibrated By	Certificate No.	Due Date
Standard Weight Class E2	1mg to 200g	B505567572	TCS	M24041005	19 April 2025

Instrument	Model	Serial No.	Calibrated By	Certificate No.	Due Date
Thermo-Hygro Meter	608-H1	NFI.BTH 017/23	Quality Reborn	QR25-0542	10 February 2026

3. This certification is traceable to SI UNIT

4. This certificate was certified only for the instrument we calibrated.

5. This result of calibration was found accurate as shown on date and place of calibration only.

**Calibration Results:**




**1. Repeatability of Reading:**

Nominal Value ( g )	Standard Deviation of Reading ( g )
40	0.0000042
80	0.0000042
100	0.000000
200	0.000000

**2. Off-Center Error:**

A mass of 100 g was placed and moved to various position on pan.

The balance reading obtained is given in the table.



1	2	3	4	5	6	(Maximum Difference)
( g )	( g )	( g )	( g )	( g )	( g )	( g )
100.0001	100.0001	100.0001	100.0001	100.0001	100.0001	0.0000

## Calibration Report

**Certificate No.:** 2502226-002-01

**Equipment:**

Electronic Balance

**Manufacturer:** METTLER TOLEDO

**Model:** XSR205DU

**Resolution:** 0.00001 g / 0.0001 g

**Serial No.:** C210685394

**ID No.:** UAE.WAO.010/2565

**Capacity:** 82 g / 220 g

**Date of Calibration:** 20 March 2025

Page 3 of 4

**Calibration Results:** (Continued)

**Calibration Range:** 0-80 g

**Calibration Adjustment:** Internal Calibration

**3. Departure from Nominal Value:** (Range: 0 - 82 g ; Resolution: 0.00001 g )

Nominal Value ( g )	Standard Value ( g )	Average Reading ( g )	Correction ( g )	Uncertainty ( ± g )	Coverage Factor k
Unload	0.000000	0.00000	0.00000	0.0000087	2.00
0.001	0.001003	0.00100	0.00000	0.0000090	2.00
0.005	0.005002	0.00501	-0.00001	0.0000092	2.00
0.01	0.010003	0.01002	-0.00002	0.0000089	2.00
0.05	0.049996	0.05001	-0.00001	0.0000096	2.00
0.1	0.100011	0.10002	-0.00001	0.000011	2.00
0.5	0.500016	0.50004	-0.00002	0.000014	2.00
1	1.000003	1.00005	-0.00005	0.000016	2.00
2	2.000023	2.00006	-0.00004	0.000017	2.00
5	5.000015	5.00006	-0.00005	0.000020	2.00
10	10.000009	10.00005	-0.00004	0.000026	2.00
20	20.000030	20.00007	-0.00004	0.000037	2.00
30	30.000039	30.00009	-0.00005	0.000050	2.00
50	50.000028	50.00008	-0.00005	0.000068	2.00
80	80.000067	80.00013	-0.00006	0.00011	2.00



## Calibration Report

**Certificate No.:** 2502226-002-01

**Equipment:**

Electronic Balance

**Manufacturer:** METTLER TOLEDO

**Model:** XSR205DU

**Resolution:** 0.00001 g / 0.0001 g

**Serial No.:** C210685394

**ID No.:** UAE.WAO.010/2565

**Capacity:** 82 g / 220 g

**Date of Calibration:** 20 March 2025

Page 4 of 4

**Calibration Results:** (Continued)

**Calibration Range:** >80-200 g

**Calibration Adjustment:** Internal Calibration

**3. Departure from Nominal Value:** (Range: >80 - 200 g ; Resolution: 0.0001 g )

Nominal Value ( g )	Standard Value ( g )	Average Reading ( g )	Correction ( g )	Uncertainty ( ± g )	Coverage Factor k
90	90.00010	90.0002	-0.0001	0.00015	2.00
100	100.00006	100.0001	0.0000	0.00016	2.00
110	110.00007	110.0002	-0.0001	0.00017	2.00
120	120.00009	120.0002	-0.0001	0.00018	2.00
130	130.00010	130.0002	-0.0001	0.00019	2.00
140	140.00013	140.0002	-0.0001	0.00019	2.00
150	150.00009	150.0002	-0.0001	0.00021	2.00
160	160.00010	160.0002	-0.0001	0.00022	2.00
170	170.00012	170.0002	-0.0001	0.00023	2.00
200	200.00013	200.0002	-0.0001	0.00028	2.00

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor  $k$ , providing a level of confidence of approximately 95 %.

----- End -----

F-CS-012 Revision: 01 Date: 20-04-65


## Calibration Certificate

**Certificate No.:** 2502226-001-01  
**Client name:** UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.  
**Address:** 3 Soi Udomsuk 41, Sukhumvit Road,  
Bangchack, Prakhnong, Bangkok 10260

Page 1 of 4

**Equipment:** Electronic Balance  
**Manufacturer:** METTLER TOLEDO  
**Model:** XSR205DU  
**Serial No.:** C009071872  
**ID No.:** UAE.WAO.012/2563  
**Order No.:** 2502226  
**Operation No.:** 2502226-001  
**Date of Receipt:** 19 March 2025  
**Date of Calibration:** 20 March 2025

**Calibrated by** Mr.Yothin Charoensuk  
Scientist

**Approved by**   
( Mr.Pheraphat Tuanjit )  
Manager, Division of Calibration Laboratory  
Responsible for the Technical Management Team

**Date of Issue:** 25 March 2025

**The uncertainties are for a confidence probability of approximately 95%**

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the National Food Institute.

FCS-009 Revision: 01 Date: 20-04-65

## Calibration Report

**Certificate No.:** 2502226-001-01

**Equipment:**

Electronic Balance

**Manufacturer:** METTLER TOLEDO

**Model:** XSR205DU

**Resolution:** 0.00001 g / 0.0001 g

**Serial No.:** C009071872

**ID No.:** UAE.WAO.012/2563

**Capacity:** 82 g / 220 g

**Date of Calibration:** 20 March 2025

Page 2 of 4

**Environment Condition:** Ambient Temperature:  $21.2 \pm 0.6$  °C Relative Humidity:  $48 \pm 3.5$  %

**Place of Calibration:** 208 Balance Room, UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.

**Condition of Equipment:** Good Condition

**Condition of This Results of Calibration:**

1. Calibration Method: NFI Method W-MA-001 In-House Method based on UKAS Lab 14 : 2019

2. Reference Standards:

Reference Standard	Model	Serial No.	Calibrated By	Certificate No.	Due Date
Standard Weight Class E2	1mg to 200g	8505567572	TCS	M24041005	19 April 2025

Instrument	Model	Serial No.	Calibrated By	Certificate No.	Due Date
Thermo-Hygro Meter	608-H1	NFI.BTH 017/23	Quality Reborn	QR25-0542	10 February 2026

3. This certification is traceable to SI UNIT

4. This certificate was certified only for the instrument we calibrated.

5. This result of calibration was found accurate as shown on date and place of calibration only.

**Calibration Results:**



**1. Repeatability of Reading:**

Nominal Value ( g )	Standard Deviation of Reading ( g )
40	0.0000052
80	0.0000042
100	0.0000000
200	0.0000000

**2. Off-Center Error:**

A mass of 100 g was placed and moved to various position on pan.

The balance reading obtained is given in the table.



1	2	3	4	5	6	(Maximum Difference)
( g )	( g )	( g )	( g )	( g )	( g )	( g )
100.0001	100.0001	100.0001	100.0001	100.0001	100.0002	0.0001



## Calibration Report

**Certificate No.:** 2502226-001-01

**Equipment:**

Electronic Balance

**Manufacturer:** METTLER TOLEDO

**Model:** XSR205DU

**Resolution:** 0.00001 g / 0.0001 g

**Serial No.:** C009071872

**ID No.:** UAE.WAO.012/2563

**Capacity:** 82 g / 220 g

**Date of Calibration:** 20 March 2025

Page 3 of 4

**Calibration Results:** (Continued)

**Calibration Range:** 0-80 g

**Calibration Adjustment:** Internal Calibration

**3. Departure from Nominal Value:** (Range: 0 - 82 g ; Resolution: 0.00001 g )

Nominal Value ( g )	Standard Value ( g )	Average Reading ( g )	Correction ( g )	Uncertainty ( ± g )	Coverage Factor k
Unload	0.00000	0.00000	0.00000	0.0000089	2.00
0.001	0.001003	0.00100	0.00000	0.0000092	2.00
0.005	0.005002	0.00500	0.00000	0.0000094	2.00
0.01	0.010003	0.01000	0.00000	0.0000091	2.00
0.05	0.049996	0.05000	0.00000	0.0000098	2.00
0.1	0.100011	0.10000	0.00001	0.000011	2.00
0.5	0.500016	0.50000	0.00002	0.000014	2.00
1	1.000003	1.00001	-0.00001	0.000016	2.00
2	2.000023	2.00005	-0.00003	0.000017	2.00
5	5.000015	5.00005	-0.00003	0.000021	2.00
10	10.000009	10.00005	-0.00004	0.000026	2.00
20	20.000030	20.00012	-0.00009	0.000037	2.00
30	30.000039	30.00012	-0.00008	0.000050	2.00
50	50.000028	50.00014	-0.00011	0.000068	2.00
80	80.000067	80.00020	-0.00013	0.00011	2.00



## Calibration Report

**Certificate No.:** 2502226-001-01

**Equipment:**

Electronic Balance

**Manufacturers:** METTLER TOLEDO

**Model:** XSR205DU

**Resolution:** 0.00001 g / 0.0001 g

**Serial No.:** C009071872

**ID No.:** UAE.WAO.012/2563

**Capacity:** 82 g / 220 g

**Date of Calibration:** 20 March 2025

Page 4 of 4

**Calibration Results:** (Continued)

**Calibration Range:** >80-200 g

**Calibration Adjustment:** Internal Calibration

**3. Departure from Nominal Value:** (Range: >80 - 200 g ; Resolution: 0.0001 g )

Nominal Value ( g )	Standard Value ( g )	Average Reading ( g )	Correction ( g )	Uncertainty ( ± g )	Coverage Factor k
90	90.00010	90.0002	-0.0001	0.00015	2.00
100	100.00005	100.0001	0.0000	0.00016	2.00
110	110.00007	110.0001	0.0000	0.00017	2.00
120	120.00009	120.0002	-0.0001	0.00018	2.00
130	130.00010	130.0002	-0.0001	0.00019	2.00
140	140.00013	140.0002	-0.0001	0.00019	2.00
150	150.00009	150.0002	-0.0001	0.00021	2.00
160	160.00010	160.0002	-0.0001	0.00022	2.00
170	170.00012	170.0002	-0.0001	0.00023	2.00
200	200.00013	200.0002	-0.0001	0.00028	2.00

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor  $k$ , providing a level of confidence of approximately 95 %.

----- End -----

F-CS-012 Revision: 01 Date: 20-04-65



01101111

## เอกสารไม่ควบคุม

## Calibration Report

**Certificate No.:** 2503287-001-01  
**Equipment:** Autoclave  
Model: CL-40L Serial No.: 810010  
Resolution: 1 °C ID No.: UAE.MIC.032/2565  
Manufacturer: ALP  
**Date of Calibration:** 5 June 2025

Page 2 of 3

**Location:** Room 301 Media Preparation, UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.  
**Environment Condition:** Ambient Temperature ( 26 ± 1 ) °C  
Relative Humidity ( 55 ± 5 ) %  
Line Voltage ( 230 ± 5 ) Volt

### Condition of this results of Calibration:

- This instrument was calibrated by insert 3 standard Data loggers with RTD into its autoclave and calibration according to W-TE-018 based on BS 2646-1:2021, Autoclaves for sterilization in laboratories  
Part 1: Design, construction, safety and performance - Specification.  
- The temperature scale used was based on ITS - 90.  
- All data show below were final values and the initial data may be obtained upon request.

### 2. Reference Standard Instrument :


Instrument	Model	Serial No.	Certificate No.	Due Date	Through
Digital Thermometer with RTD (Data Logger)	HiTemp140-PT	T20627	NC-25-03-18-181	11-Mar-26	MADGETECH, INC.
	OM-CP-HITEMP-140	R56916	2502081-002-01	11-Mar-26	NATIONAL FOOD INSTITUTE
	PRTemp140	R38546	2501835-001-01	22-Feb-26	NATIONAL FOOD INSTITUTE

- This certificate is traceable to International System of Units (SI Units).
- This certificate was certified only for the instrument we calibrated.
- This result of calibration was found accurate as shown on date and place of calibration only.
- This standard does not apply to sterilizers or disinfectors used for medical, dental, pharmaceutical.
- Condition of Calibrated item : Good

UUC Description : Setting program function sterilization : STERILIZE/NORMAL

Time of sterilization 20 Minute At 115 and 121 °C

8. Result of Calibration :
- |                                     |                    |
|-------------------------------------|--------------------|
| <input checked="" type="checkbox"/> | Without adjustment |
| <input type="checkbox"/>            | After adjustment   |

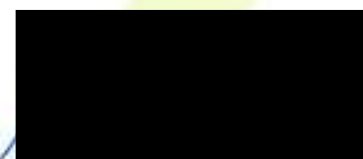

11 June 2025





## Calibration Report

Certificate No.: 2503287-001-01

Equipment: Autoclave

Model: CL-40L

Serial No.: 810010

Resolution: 1 °C

ID No.: UAE.MIC.032/2565

Manufacturer: ALP


Date of Calibration: 5 June 2025

Page 3 of 3

Calibration point: 115 and 121 °C

Calibration result:

Calibration Condition	Temperature (°C)	Relative Humidity (%)	Line Voltage (Volt)
Min	25.8	50	225
Max	26.8	59	235

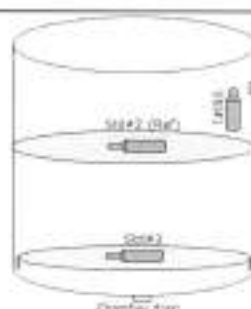

Standard at Pressure

Sensor 1 is attached to the test temperature probe, within 30 min.  
Sensor 2 is in the upper half of the chamber, within 30 min.  
Sensor 3 is in the chamber door, within 30 min.

Table 1 : Reporting of Temperature

Calibration Point (°C)	Measured Temperature (°C) @ Sensor No. (Sensor No.2 is REF)			Uncertainty ± (°C)
	Std. # 1	Std. # 2 (Ref)	Std. # 3	
115	115.46	115.43	115.42	0.70
121	121.59	121.54	121.51	0.70

Table 2 : Reporting of Characterization Result

UUC* Setting (°C)	UUC* Reading				Stability ± (°C)	Uniformity (°C)	Overall Variation (°C)
	Min (°C)	Max (°C)	Average (°C)	MPa			
115	115	115	115	0.08	0.24	0.17	0.50
121	121	121	121	0.12	0.24	0.19	0.52

### Note

The quoted uncertainty include " Stability " and " Loading effect ( 20% of Uniformity )"

UUC\* = Unit Under Calibration

Stability = One-half of the greatest maximum difference of measured temperatures at any one sensors, for at least half an hour after reaching steady state.

Uniformity = The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time.

Overall Variation = The difference of the maximum and minimum measured temperatures throughout observation time.

The report uncertainty of measurement was based on standard uncertainty multiplied by coverage factor k= 2, providing a level of confidence of approximately 95 %.

----- End -----







TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)  
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES  
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250  
TEL.0-2717-3000-29 FAX.0-2719-9484



## Certificate of Calibration

Cert. No.: 25TM577

Page : 1 of 3

Equipment : BOD Incubator

Manufacturer : ARCO

Model : UR-1320

Serial No. : -

ID No. : UAE.WAO.018/2551

Submitted by : United Analyst and Engineering Consultant Co.,Ltd.  
3 Soi Udomsuk 41, Sukhumvit Road,  
Bangchak, Phrakhanong,  
Bangkok 10260

Location : Lab Floor 2

Received Order : 19 March 2025

Calibration Date : 19 March 2025

Ambient Temperature :  $(26 \pm 10) ^\circ\text{C}$

Relative Humidity :  $(50 \pm 30) \%$

AC Line Voltage :  $(220 \pm 22) \text{ V}$

Calibrated by : Man Pattanapongpalboon

Approved by :

Approved Signatory

( ) Chakrit Waewwanjua  
( ) Suwit Imjai  
(✓) Kunchit Promprat

Issue Date : 27 March 2025

**The Uncertainties are for a confidence probability of approximately 95%**

This certificate may not be reproduced other than in full, except with the prior written  
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

เอกสารไม่ควบคุม



Equipment : BOD Incubator  
Condition As-Received : Used Item  
Reference : 2503-0437OC-1

Cert. No.: 25TM577

Page : 2 of 3

**Procedure Used :-**

Calibration were conducted using calibration procedure CP-OT02 based on TLAS G-20 according to direct measurement method with Data Acquisition which connected with Resistance Temperature Detector ( RTD ).

The temperature scale used was based on ITS-90.

**Condition of this result of calibration**

**1. Reference standard instrument:-**

Instrument	Serial No.	Cert. No.	Traceable	Due Date
1 ) Data Acquisition	MY57013823	24LM71	TPA	12 May 2025

2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certification is traceable to the International System of Unit.


**Remark :** TPA : Technology Promotion Association ( Thailand - Japan )

**Result of Calibration :-** ( \* ) Without Adjustment

**Function of UUC\* :** Temperature Source

**Fresh air setting :** Close

Environment during calibration		
	Beginning	Finished
Temp. ( °C )	28	28
REL.Humid. ( % )	56	55
AC Supply ( Volt )	224	224

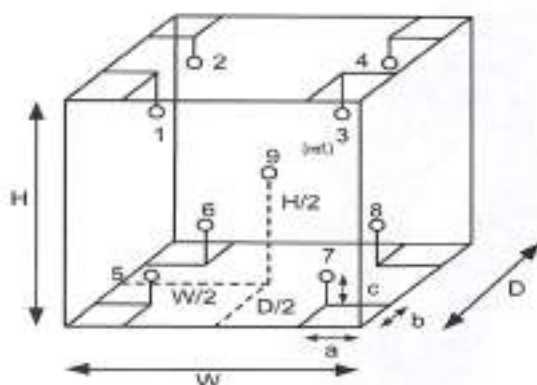

Position :	Ref. Std. ID No.:
1	21-17RTD-01
2	21-17RTD-02
3	17RTD-03
4	24-17RTD-04
5	17RTD-05
6	17RTD-06
7	17RTD-07
8	23-17RTD-08
9 (ref.)	23-17RTD-09

**Probe Installation Details :**

a = 10 cm  
b = 10 cm  
c = 10 cm

**Dimension of Chamber :**

D = 0.62 m  
W = 1.2 m  
H = 1.2 m  
Capacity = 0.89 m<sup>3</sup>

เอกสารไม่ควบคุม



Equipment : BOD Incubator  
Condition As-Received : Used Item  
Reference : 2503-0437OC-1  
Result of Calibration :- ( \* ) Without Adjustment  
Function of UUC\* : Temperature Source  
Fresh air setting : Close

Cert. No.: 25TM577

Page : 3 of 3

Calibration Point ( °C )	UUC* Setting ( °C )	UUC* Reading ( °C )	Temperature stability ( ± °C )	Temperature uniformity ( °C )	Overall Variation ( °C )	Coverage Factor <i>k</i>
20.0	20.0	20.0	0.24	0.54	0.99	2

Calibration Point ( °C )	Measured Temperature ( °C )									Uncertainty  ( ±°C )
	Position									
	1	2	3	4	5	6	7	8	9 (ref.)	
20.0	20.215	20.192	19.652	19.710	19.710	20.006	19.720	19.810	19.733	0.41

**Average\*** : The average of 30 values in each position.

**Temperature stability** : One-half of the greatest maximum difference of measured temperature at any one sensor.

**Temperature uniformity** : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.

**Overall Variation** : The Difference of the maximum and minimum measured temperatures throughout observation.

**UUC\*** : Unit Under Calibration

**Note** : The reported uncertainty of measurement was included stability and excluded uniformity .

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

เอกสารไม่ควบคุม





**TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)**  
**CORPORATE SERVICES 3 : EQUIPMENT CALIBRATION AND TESTING SERVICES**

534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250

TEL. 0-2717-3000 FAX. 0-2719-9484

## Certificate of Testing

Cert.No.: 25TW29

Page.: 1 of 2

**Equipment :** DO Meter

**Manufacturer :** YSI

**Model :** 5100

**Serial No. :** 11B 101863

**ID No. :** UAE.WAO.004/2554

**Received Date :** 14 February 2025

**Test Date :** 17 February 2025

**Reference :** 2502-0473DSC-1

**Submitted by :** United Analyst and Engineering Consultant Co.,Ltd.  
3 Soi Udomsuk 41, Sukhumvit Road, Bangchak,  
Phrakhanong, Bangkok 10260

**Laboratory Condition :** Temperature (  $25 \pm 5$  ) °C  
Humidity (  $50 \pm 20$  ) %

**Test Procedure :** In - house method : CP-CH9  
by Comparison Technique with Azide Modification Method

**Tested by :** Walalak Sirithean

**Approved by :**   
Approved Signatory

( ) Chakrit Waewwanjua  
( ) Ponpan Paipim  
(✓) Salthip Meangmai

**Issue Date :** 18 February 2025

เอกสารไม่ควบคุม





Cert.No.: 25TW29

Page.: 2 of 2

**Condition of this result of calibration**

**1. Reference Standard Instruments :**

This certification is traceable to the International System of Unit through the reference standards laboratory of Industrial Calibration Center, Technology Promotion Association (Thailand-Japan).

<u>Instruments</u>	<u>Serial No.</u>	<u>ID No.</u>	<u>Certificate No.</u>	<u>Due Date</u>
1. Burette	-	130BU10	23CG1172	22 Mar 2025
2. Balance	14233821	110RC001	24MM131	04 July 2025

**2. Standard Material :-**

<u>Material</u>	<u>Manufacturer</u>	<u>Lot.No.</u>	<u>Assay</u>
Sodium Thiosulfate 5-Hydrate AR	KEMAUS	2203162447	99.6%

**Result :**            **Dissolved Oxygen Meter Adjustment With Air 100 %**  
                             **Dissolved Oxygen Probe No.: 24F100202**

<b>Titration Method (Azide Modification Method) (mg/L)</b>	<b>DO Meter Reading (mg/L)</b>	<b>Standard Deviation (mg/L)</b>
8.22	8.22	0.0055

This report was certified only for the instrument we tested. It is allowable to use for study  
Intend to use for advertising and referral purpose is prohibited. This report may not be reproduced  
other in full, without written approval of the laboratory

-o0o-

เอกสารไม่ควบคุม

บันทึกผลการตรวจสอบใบรับรองการสอบเทียบ (Verification of Certificate)

Certificate No. : 25TW29				Equipment : Do Meter			
Brand : YSI				Model : 5100			
Serial No. : 118 101863				ID No. : UAE WAO.004/2554			
Calibration results							
Titration Method	Standard Deviation	Do meter Reading	Error%	Correction%	Error   Total Error	Judgement	(Total Error < Judgement )
( mg/L)	( mg/L)	( mg/L)	( mg/L)	( mg/L)	( mg/L)	(± mg/L)	( mg/L)
8.22	0.0055	8.22	0.0000	0.0000	0.0	0.02	pass
ผู้บันทึก.....ผู้ตรวจ.....							
วันที่.....28/02/2025.....วันที่.....28 ก.พ. 68.....							
หน่วยงาน.....							

หน้า 1 จาก 1

\*\*\*\*\*

เอกสารไม่ควบคุม


## Verification Certificate

**Certificate No.:** 2501440-001-01  
**Client name:** UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.  
**Address:** 3 Soi Udomsuk 41, Sukhumvit Road,  
 Bangchack, Prakhnong, Bangkok 10260

Page 1 of 4

**Equipment:** Digestion Unit (Heating Block)  
**Manufacturer:** FOSS  
**Model:** Tecator Digestor 2520  
**Serial No.:** 91905060  
**ID No.:** UAE.WAS.030/2566  
**Order No.:** 2501440  
**Operation No.:** 2501440-001  
**Date of Receipt:** 27 January 2025  
**Date of Calibration:** 27 January 2025

**Calibrated by** Mr.Worapob Sookthong  
 Scientist

**Approved by**   
 ( Mr.Pheraphat Tuanjit )  
 Manager, Division of Calibration Laboratory  
 Responsible for the Technical Management Team

**Date of Issue:** 29 January 2025

**The uncertainties are for a confidence probability of approximately 95 %.**

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the National Food Institute.

F-CS-009 Revision: 01 Date: 20-04-65

## Verification Report

**Certificate No.:** 2501440-001-01  
**Equipment:** Digestion Unit (Heating Block)  
Model: Tecator Digestor 2520 Serial No.: 91905060  
Resolution: 1 °C ID No.: UAE.WAS.030/2566  
Manufacturer: FOSS  
**Date of Calibration:** 27 January 2025

Page 2 of 4

**Location:** Dry Laboratory (312), UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.  
**Environment Condition:** Ambient Temperature ( 29 ± 1 ) °C  
Relative Humidity ( 58 ± 2 ) %  
Line Voltage ( 224 ± 1 ) Volt

### Condition of this results of Calibration:

- This instrument was calibrated by insert standard thermocouples type R into its Digestion blocks and Calibration according to NFI Method W-TE-026 based on BS 4309 : 1968
  - The temperature scale used was based on ITS - 90 .
  - All data show below were final values and the initial data may be obtained upon request.

### 2. Reference Standard Instrument :

Instrument	Model	Serial No.	Certificate No.	Due Date	Through
Digital Thermometer with Thermocouple	34970A	MY4045575/MY41194453	TC24/0063	5-Jun-2025	N.M. Technical Center Laboratory
	Type R	S/CH1, R/CH2, R/CH3			

- This certificate is traceable to International System of Units (SI Units).
- This certificate was certified only for the instrument we calibrated.
- This result of calibration was found accurate as shown on date and place of calibration only.
- Condition of Calibrated item : Good

UUC\* Description

Time of Record 1 Hour 6 Minute At 380 °C

7. Result of Calibration : ☒ Without adjustment ☐ After adjustment



## Verification Report

**Certificate No.:** 2501440-001-01  
**Equipment:** Digestion Unit (Heating Block)  
Model: Tecator Digestor 2520 Serial No.: 91905060  
Resolution: 1 °C ID No : UAE.WAS.030/2566  
Manufacturer: FOSS

**Date of Calibration:** 27 January 2025

Page 3 of 4

**Calibration point:** 380 °C

**Calibration result:**

**Table1 : Reporting of Temperature**

Block No.	UUC* Setting (°C)	UUC* Reading (°C)	Stability (±°C)	Standard Thermometer (°C)	Uncertainty (±°C)
1	380	380	0.22	377.84	2.0
2	380	380	0.19	378.68	2.0
3	380	380	0.13	378.70	2.0
4	380	380	0.12	379.82	2.0
5	380	380	0.20	381.01	2.0
6	380	380	0.16	380.48	2.0
7	380	380	0.16	378.22	2.0
8	380	380	0.19	377.99	2.0
9	380	380	0.09	378.48	2.0
10	380	380	0.15	378.17	2.0
11	380	380	0.18	377.64	2.0
12	380	380	0.11	379.27	2.0
13	380	380	0.13	378.14	2.0
14	380	380	0.25	379.11	2.0
15	380	380	0.15	379.83	2.0
16	380	380	0.18	378.05	2.0
17	380	380	0.31	378.44	2.0
18	380	380	0.18	378.29	2.0
19	380	380	0.17	378.41	2.0
20	380	380	0.13	379.24	2.0

**Note:**

- UUC\* = Unit Under Calibration
- Immersion depth of standard thermometer in tube level high of sand is equal heater plate of UUC.
- Stability = One-half of the greatest maximum difference of measured temperatures at one sensors, for at least half an hour after reaching steady state.

The report uncertainty of measurement was based on standard uncertainty multiplied by coverage factor  $k=2$ , providing a level of confidence of approximately 95 %.



# Calibration Certificate

**Certificate No.:** 2503682-004-01

**Client name:** UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.

**Address:** 3 Soi Udomsuk 41, Sukhumvit Road,  
Bangchack, Prakhonong, Bangkok 10260

Page 1 of 3

**Equipment:** CHAMBER (Incubator)

Manufacturer: BINDER

Model: KB 400

Serial No.: 20220000022479

ID No.: UAE.MIC.028/2566

Order No.: 2503682

Operation No.: 2503682-004

**Date of Receipt:** 1 July 2025

**Date of Calibration:** 1 July 2025

**Calibrated by** Mr.Pheraphat Tuanjit  
Scientist

Approved by [Redacted]  
( Miss Preeyaporn Jaengkarnkit )  
Vice President, Department of Laboratory Services  
Responsible for the Technical Management Team

Date of Issue: 3 July 2025

The uncertainties are for a confidence probability of approximately 95 %.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the National Food Institute.

F-C5-009 Revision: 01 Date: 20-04-65



## Calibration Report

**Certificate No.:** 2503682-004-01  
**Equipment:** CHAMBER (Incubator)  
Model: KB 400 Serial No.: 20220000022479  
Resolution: 0.1 °C ID No.: UAE.MIC.028/2566  
Manufacturer: BINDER  
**Date of Calibration:** 1 July 2025

Page 2 of 3

**Location:** Microbiology Laboratory, UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.  
**Environment Condition:** Ambient Temperature ( 21 ± 1 ) °C  
Relative Humidity ( 55 ± 10 ) %  
Line Voltage ( 230 ± 5 ) Volt

### Condition of this results of Calibration:

- This instrument was calibrated by insert 13 standard thermometer into its chamber and calibration according to W-TE-014 Based on TLAS G-20-1/02-08 (E): Guidelines for Calibration and Checks of Temperature Controlled Enclosures.  
- The temperature scale used was based on ITS - 90.  
- All data show below were final values and the initial data may be obtained upon request.

### 2. Reference Standard Instrument :

Instrument	Model	Serial No./ID No.	Certificate No.	Due Date	Through
Digital Thermometer with sensor	34972A	MY59003377	2501168-001-01	13 January 2026	NATIONAL FOOD INSTITUTE
	RTD	CH#101-203 / RTD#101-203			

- This certificate is traceable to International System of Units (SI Units).
- This certificate was certified only for the instrument we calibrated.
- This result of calibration was found accurate as shown on date and place of calibration only.
- Condition of Calibrated item : Good

### UUC Description :

Time of Record 1 Hour 9 Minute At 35.0 °C  
Fresh air Damper - Open Position -  
X Close Fan 100%  
- Not Available

7. Result of Calibration : ☒ Without adjustment ☐ After adjustment



## Calibration Report

**Certificate No.:** 2503682-004-01  
**Equipment:** CHAMBER (Incubator)  
**Model:** KB 400 **Serial No.:** 20220000022479  
**Resolution:** 0.1 °C **ID No.:** UAE.MIC.028/2566  
**Manufacturer:** BINDER

**Date of Calibration:** 1 July 2025

Page 3 of 3

**Calibration point:** 35.0 °C

**Calibration result:**

Calibration Condition	Temperature (°C)	Relative Humidity (%)	Line Voltage (Volt)
MIN	20.1	45	225.0
MAX	22.0	65	235.0

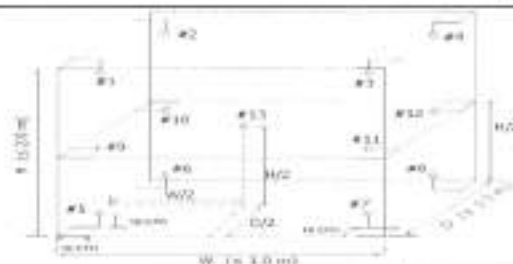


Table 1 : Reporting of Temperature

Calibration point (°C)	Measured Temperature (°C) @ Sensor No. (Sensor No.13 is REF)													Uncertainty ± (°C)
	# 1	# 2	# 3	# 4	# 5	# 6	# 7	# 8	# 9	# 10	# 11	# 12	# 13	
35.0	35.19	35.03	34.83	35.21	34.96	34.94	34.84	34.84	35.06	34.94	35.15	34.79	34.92	0.27

Table 2 : Reporting of Characterization Result

UUC* Setting (°C)	UUC* Reading (°C)			Temperature Stability ± (°C)	Temperature Uniformity (°C)	Overall Variation (°C)
	MIN	MAX	Average			
34.8	34.8	34.8	34.8	0.040	0.29	0.50

**Note** The quoted uncertainty include " Stability " and " Loading effect (20% of Temp Uniformity) "

UUC\* = Unit Under Calibration

Stability = One-half of the greatest maximum difference of measured temperatures at any one sensors, for at least half an hour after reaching steady state.

Uniformity = The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time.

Overall Variation = The difference of the maximum and minimum measured temperatures throughout observation time.

The report uncertainty of measurement was based on standard uncertainty multiplied by coverage factor  $k=2$ , providing a level of confidence of approximately 95 %.

----- End -----

3 July 2025

เอกสารไม่ควบคุม




## Calibration Certificate

**Certificate No.:** 2502229-002-01  
**Client name:** UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.  
**Address:** 3 Soi Udomsuk 41, Sukhumvit Road,  
Bangchack, Prakanong, Bangkok 10260

Page 1 of 3

**Equipment:** CHAMBER (Incubator)  
**Manufacturer:** MEMMERT  
**Model:** IPP260  
**Serial No.:** V616.0066  
**ID No.:** UAE.MIC.032/2559  
**Order No.:** 2502229  
**Operation No.:** 2502229-002  
**Date of Receipt:** 19 March 2025  
**Date of Calibration:** 19 March 2025

**Calibrated by** Mr.Yothin Charoensuk  
Scientist

**Approved by**   
( Mr.Pheraphat Tuanjit )  
Manager, Division of Calibration Laboratory  
Responsible for the Technical Management Team

**Date of Issue:** 25 March 2025

The uncertainties are for a confidence probability of approximately 95 %.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the National Food Institute.

F-CS-009 Revision: 01 Date: 20-04-65

เอกสารไม่ควบคุม











# FOSS

FOSS South East Asia

3388 Sirinrat Building, 25th - 26th Floor, Unit No. 3388/90,  
Rama IV Road, Klongton, Klongtoey, Bangkok, Thailand 10110

## Customer Service Report

Report No.:

13319

Date:

Jan 27, 2025

Customer:

UAE

Job No.:

11675

Address:

Bangkok

Instrument:

KT200

Serial:

91790524

Start  
Finish

Travel To Customer (Hrs)

09.00

10.00

1

Labour (Hrs)

10.00

13.00

3

Travel From Customer (Hrs)

-

-

### Job Type

Application	Special	Standard
Distributor	Courtesy Visit	Installation
Digital Service	PMA Onboarding	Quote
Internal	Warranty	Repair
Investigate	Sales Support	Remote
		Training
		In House
		PM
		Health Check Visit

PMA Type

Smartcare

x

Smartcare Pro

x

Fosscore

x

Smartcare Advance

x

Fosscore Pro

x

N/A

x

### Details of Work / Test

- PM -	
+ Visual Check	
- No leak	- ok
- have damage on heater & main switch	- Not ok
+ replace heater & main switch	- ok
+ replace PM kit #1 set	- ok
+ Function Check	
- Power on / off	- ok
- Alarm	- ok
- Steam	- ok
- Condenser	- ok
- Water pump	- ok
Instrument Ready for Use	OK
	30
	Not OK*
	x

Part No.	Batch	Description	Qty
100159965	11-06-2024	FOSS PM kit KT200 bfilter Analyser / 210g	1
10003512	29.03.2024	Heating element Steam	1
15630111	19.10.2022	Switch R595kit + 2 pin	1

I confirm this report is accurate and complete

Signed FOSS		Signed Customer	
Name		Name	

Email:

Customer Contact.:

\*Remark:

เอกสารไม่ควบคุม



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)  
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES  
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250  
TEL.0-2717-3000-29 FAX.0-2719-9484



## Certificate of Calibration

Cert.No.: 25CH861

Page.: 1 of 3

Equipment :	pH Meter
Manufacturer :	YSI
Model :	pH100A
Serial No. :	JC02729
ID No. :	UAE.EFM 1957561 (ENV.pH 04/61)
Condition As-Received:	Used Item
Received Date :	22 July 2025
Calibration Date :	23 July 2025
Reference :	2507-0753WSC-1
Submitted by :	United Analyst and Engineering Consultant Co.,Ltd. 3 Soi Udomsuk 41, Sukhumvit Road, Bangkok, Phrakhanong, Bangkok 10260
Ambiant Temperature :	(25 ± 2.5) °C
Relative Humidity :	(50 ± 15) %
Calibration Procedure :	In - house method : - CP-CH5 by direct measurement with DC voltage standard and direct measurement with certified reference material (CRM) - CP-CH8 by comparison with temperature standard
Calibrated by :	Walalak Sirithuan 
Approved by :	 Approved Signatory
	<input type="checkbox"/> Chakrit Waeuwwanjua <input type="checkbox"/> Ponpan Paipim <input checked="" type="checkbox"/> Salthip Meangma
Issue Date :	24 July 2025

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written  
Approval of the head of Corporate Services 3: Equipment Calibration and Testing Services

เอกสารไม่ควบคุม



Cert.No.: 25CH861

Page.: 2 of 3

**Condition of this calibration result**

**1. Reference Standard Instrument**

<u>Instrument</u>	<u>Serial No.</u>	<u>ID No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
1) Document Process Calibrator	54030049	130RC116	24E275B	25 Aug 2025
2) Ref. Standard Thermometer	4982054	110RC044	25170B	03 July 2028

- This measurement result is traceable to SI through Technology Promotion Association (Thailand - Japan)

- 2. Certified Reference Materials** :The measurement results are traceable to SI through Hach Lange GmbH Ltd.  
Deutsche Akkreditierungsstelle, Accredited No.D-RNA-15184-01-30  
;The measurement results are traceable to SI through CPA chem Ltd  
ANSI-ASQ National Accreditation Board, Accredited No. AB-1835

<u>Buffer Solution</u>	<u>Manufacturer</u>	<u>Lot No.</u>	<u>Exp. date</u>
pH 4.007	CPA chem	1056665	18 Jan 2027
pH 7.000	Hach Lange GmbH	C03232	02 Dec 2026
pH 10.010	CPA chem	1114385	08 June 2026

3. This certificate is valid only to the item calibrated on date and place of calibration.

**Calibration Results**

**Function :** mV Measurement

**Performing standard curve by Document Process Calibrator at pH (4,7)(7,10)**

Unit Under Calibration	Nominal Value	Standard Voltage Input	Actual Reading		Uncertainty of Measurement { ±mV }	Coverage factor k
	pH	mV	mV	pH		
pH Meter S/N.: JC02728	4.00	177.48	177	4.01	0.58	2.00
	7.00	0.00	0	7.00	0.58	2.00
	7.00	0.00	0	7.00	0.58	2.00
	10.00	-177.48	-177	10.01	0.58	2.00

เอกสารไม่ควบคุม



Cert.No.: 25CH881

Page.: 3 of 3

**Calibration Results****Function : pH Measurement****Performing three buffers standard curve by using buffer nominal pH (4,7)(7,10)**

Unit Under Calibration	Standard pH Buffer Solution	Actual pH Reading	Actual mV Reading (mV)	Uncertainty of pH Measurement ( $\pm$ )	Coverage factor $k$
pH Electrode S/N.: 2403D4SIA605377	4.007	4.01	171	0.0079	2.00
	7.000	6.99	-3	0.0095	2.00
	7.000	7.00	-3	0.0092	2.00
	10.010	10.00	-174	0.0095	2.00

**Function : Temperature Measurement****(\*) Without adjustment**

This equipment was connected with Temperature Probe:

- Model :

-

- Serial No. :

240904SIA605377

Dimension of probe

- Length :

110 mm

- Diameter :

12 mm.

- Immersion Depth :

100 mm.

Calibration Point ( $^{\circ}\text{C}$ )	Standard Temperature ( $^{\circ}\text{C}$ )	UUC* Reading ( $^{\circ}\text{C}$ )	Error ( $^{\circ}\text{C}$ )	Uncertainty of measurement ( $\pm$ $^{\circ}\text{C}$ )	Coverage factor $k$
15.0	15.002	14.9	-0.102	0.13	2.00
30.0	30.002	30.0	-0.002	0.13	2.00
45.0	45.003	44.9	-0.103	0.13	2.00

**Remark** - UUC\* = Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor  $k$ , providing a level of confidence of approximately 95 %.

-o0o-

เอกสารไม่ควบคุม





TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)  
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES  
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250  
TEL.0-2717-3000-29 FAX.0-2719-9484



## Certificate of Calibration

Cert. No.: 25TM501

Page : 1 of 3

Equipment : Water Bath

Manufacturer : Memmert

Model : WNE 14

Serial No. : L414.1407

ID No. : UAE.MIC.006/2558

Submitted by : United Analyst and Engineering Consultant Co.,Ltd.  
3 Soi Udomsuk 41, Sukhumvit Road,  
Bangchak, Phrakhanong,  
Bangkok 10260

Location : Microbiology Laboratory (302)

Received Order : 19 March 2025

Calibration Date : 19 March 2025

Ambient Temperature :  $( 26 \pm 10 ) ^\circ\text{C}$

Relative Humidity :  $( 50 \pm 30 ) \%$

AC Line Voltage :  $( 220 \pm 22 ) \text{ V}$

Calibrated by : Krisda Malee

Approved by :   
Approved Signatory

☐ Chakrit Waewwanjua

☐ Suwit Imjai

☒ Kunchit Promprat

Issue Date : 27 March 2025

**The Uncertainties are for a confidence probability of approximately 95%**

This certificate may not be reproduced other than in full, except with the prior written  
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

เอกสารไม่ควบคุม



**Equipment :** Water Bath  
**Condition As-Received :** Used Item  
**Reference :** 2503-0436OC-1  
**Procedure Used :-**

**Cert. No.:** 25TM501  
**Page :** 2 of 3

Calibration were conducted using in-house calibration procedure CP-OT04 Based on ASTM E715 according to direct measurement method with Data Acquisition which connected with Industrial Platinum Resistance Thermometer ( IPRT ).

The temperature scale used was based on ITS-90.

**Condition of this result of calibration**

1. Reference standard instrument:-

<u>Instrument</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Traceable</u>	<u>Due Date</u>
1 ) Data Acquisition	MY57013823	23LM71	TPA	12 May 2025

2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certification is traceable to the International System of Unit.


**Remark :** TPA : Technology Promotion Association ( Thailand - Japan )

**Result of Calibration :-** ( \* ) Without Adjustment

**Function of UUC\* :** Temperature Source

**Heat transfer medium used :** Water

	<u>Environmental</u>		<u>AC Voltage Supply</u>
	( °C )	( %R.H. )	( Volt )
Beginning of Calibration	24	50	220
Finished of Calibration	25	53	221

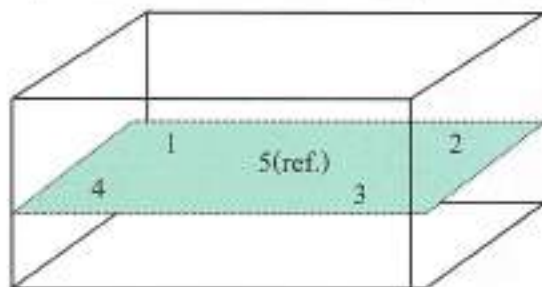

Front

<u>Position :</u>	<u>Ref. Std. S/N.:</u>
1	4804539-006
2	4804539-007
3	4804539-008
4	4804539-009
5(ref.)	4804539-010



Equipment : Water Bath  
Condition As-Received : Used Item  
Reference : 2503-0436OC-1  
Result of Calibration :- ( \* ) Without Adjustment  
Function of UUC\* : Temperature Source

Cert. No.: 25TM501

Page : 3 of 3

Calibration point ( °C )	UUC* Setting ( °C )	UUC* Reading ( °C )	Average* Standard Reading ( °C )					Uncertainty  ( ± °C )
			Position					
			1	2	3	4	5 (ref.)	
44.5	44.4	44.4	44.508	44.531	44.495	44.537	44.510	0.15

Calibration point ( °C )	Uniformity ( °C )	Stability ( ± °C )	Coverage Factor <i>k</i>
44.5	0.092	0.048	2

**Average\*** : The average of 30 values in each position.

**Uniformity** : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.

**Stability** : One-half of the greatest maximum difference of measured temperature at any one probe.

**UUC\*** : Unit Under Calibration

**Note** : The reported uncertainty of measurement was included stability and excluded uniformity.

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

เอกสารไม่ควบคุม

## List of Instrument Certificates for Environmental Quality Analysis

No.	Instrument/Equipment	Parameter	Manufacturer	Model/Serial No.	Calibrator	Certification No.	Date of Calibration	Due date of Calibration*
1	Incubator	TOTAL BACTERIA	Binder	KB400 / 20220000022479	National food institute ministry of Industry	2503682 004 01	1/7/2025	30/6/2026
2	pH Meter	pH	YSI Environmental	pH 100A / JC02729	Technology Promotion Association (Thailand-Japan)	25CH861	23/7/2025	22/7/2026

**Due Date of Calibration\*** : Based on the annual calibration plan. At least 1 time per year.



ed orth

## Calibration Report

**Certificate No.:** 2503682-004-01  
**Equipment:** CHAMBER (Incubator)  
Model: KB 400 Serial No.: 20220000022479  
Resolution: 0.1 °C ID No.: UAE.MIC.028/2566  
Manufacturer: BINDER  
**Date of Calibration:** 1 July 2025

Page 2 of 3

**Location:** Microbiology Laboratory, UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.  
**Environment Condition:** Ambient Temperature ( 21 ± 1 ) °C  
Relative Humidity ( 55 ± 10 ) %  
Line Voltage ( 230 ± 5 ) Volt

### Condition of this results of Calibration:

- This instrument was calibrated by insert 13 standard thermometer into its chamber and calibration according to W-TE-014 Based on TLAS G-20-1/02-08 (E): Guidelines for Calibration and Checks of Temperature Controlled Enclosures.  
- The temperature scale used was based on ITS - 90.  
- All data show below were final values and the initial data may be obtained upon request.

### 2. Reference Standard Instrument :

Instrument	Model	Serial No./ID No.	Certificate No.	Due Date	Through
Digital Thermometer with sensor	34972A	MY59003377	2501168-001-01	13 January 2026	NATIONAL FOOD INSTITUTE
	RTD	CH#101-203 / RTD#101-203			

- This certificate is traceable to International System of Units (SI Units).
- This certificate was certified only for the instrument we calibrated.
- This result of calibration was found accurate as shown on date and place of calibration only.
- Condition of Calibrated item : Good

### UUC Description :

Time of Record 1 Hour 9 Minute At 35.0 °C  
Fresh air Damper - Open Position -  
X Close Fan 100%  
- Not Available

7. Result of Calibration : ☒ Without adjustment ☐ After adjustment

## Calibration Report

**Certificate No.:** 2503682-004-01  
**Equipment:** CHAMBER (Incubator)  
**Model:** KB 400 **Serial No.:** 20220000022479  
**Resolution:** 0.1 °C **ID No.:** UAE.MIC.028/2566  
**Manufacturer:** BINDER

**Date of Calibration:** 1 July 2025

Page 3 of 3

**Calibration point:** 35.0 °C

**Calibration result:**

Calibration Condition	Temperature (°C)	Relative Humidity (%)	Line Voltage (Volt)
MIN	20.1	45	225.0
MAX	22.0	65	235.0

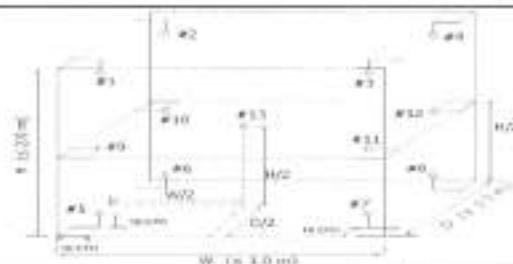


Table 1 : Reporting of Temperature

Calibration point (°C)	Measured Temperature (°C) @ Sensor No. (Sensor No.13 is REF)													Uncertainty ± (°C)
	# 1	# 2	# 3	# 4	# 5	# 6	# 7	# 8	# 9	# 10	# 11	# 12	# 13	
35.0	35.19	35.03	34.83	35.21	34.96	34.94	34.84	34.84	35.06	34.94	35.15	34.79	34.92	0.27

Table 2 : Reporting of Characterization Result

UUC* Setting (°C)	UUC* Reading (°C)			Temperature Stability ± (°C)	Temperature Uniformity (°C)	Overall Variation (°C)
	MIN	MAX	Average			
34.8	34.8	34.8	34.8	0.040	0.29	0.50

**Note** The quoted uncertainty include " Stability " and " Loading effect (20% of Temp Uniformity) "

UUC\* = Unit Under Calibration

Stability = One-half of the greatest maximum difference of measured temperatures at any one sensors, for at least half an hour after reaching steady state.

Uniformity = The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time.

Overall Variation = The difference of the maximum and minimum measured temperatures throughout observation time.

The report uncertainty of measurement was based on standard uncertainty multiplied by coverage factor  $k=2$ , providing a level of confidence of approximately 95 %.

----- End -----

3 July 2025

เอกสารไม่ควบคุม







TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)  
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES  
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250  
TEL.0-2717-3000-29 FAX.0-2719-9484



## Certificate of Calibration

Cert.No.: 25CH861

Page.: 1 of 3

Equipment :	pH Meter
Manufacturer :	YSI
Model :	pH100A
Serial No. :	JC02729
ID No. :	UAE.EFM 19527561(ENV.pH 04/61)
Condition As-Received:	Used Item
Received Date :	22 July 2025
Calibration Date :	23 July 2025
Reference :	2507-0753WSC-1
Submitted by :	United Analyst and Engineering Consultant Co.,Ltd. 3 Soi Udomsuk 41, Sukhumvit Road, Bangkok, Phrakhanong, Bangkok 10260
Ambiant Temperature :	(25 ± 2.5) °C
Relative Humidity :	(50 ± 15) %
Calibration Procedure :	In - house method : - CP-CH5 by direct measurement with DC voltage standard and direct measurement with certified reference material (CRM) - CP-CH8 by comparison with temperature standard
Calibrated by :	Walalak Sirithuan 
Approved by :	 Approved Signatory
	<input type="checkbox"/> Chakrit Waeuwwanjua <input type="checkbox"/> Ponpan Paipim <input checked="" type="checkbox"/> Salthip Meangma
Issue Date :	24 July 2025

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written  
Approval of the head of Corporate Services 3: Equipment Calibration and Testing Services

เอกสารไม่ควบคุม





Cert.No.: 25CH861

Page.: 2 of 3

**Condition of this calibration result**

**1. Reference Standard Instrument**

<u>Instrument</u>	<u>Serial No.</u>	<u>ID No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
1) Document Process Calibrator	54030049	130RC116	24E275B	25 Aug 2025
2) Ref. Standard Thermometer	4982054	110RC044	25170B	03 July 2028

- This measurement result is traceable to SI through Technology Promotion Association (Thailand - Japan)

- 2. Certified Reference Materials** :The measurement results are traceable to SI through Hach Lange GmbH Ltd.  
Deutsche Akkreditierungsstelle, Accredited No.D-RNA-15184-01-30  
;The measurement results are traceable to SI through CPA chem Ltd  
ANSI-ASQ National Accreditation Board, Accredited No. AB-1835

<u>Buffer Solution</u>	<u>Manufacturer</u>	<u>Lot No.</u>	<u>Exp. date</u>
pH 4.007	CPA chem	1056665	18 Jan 2027
pH 7.000	Hach Lange GmbH	C03232	02 Dec 2026
pH 10.010	CPA chem	1114385	08 June 2026

3. This certificate is valid only to the item calibrated on date and place of calibration.

**Calibration Results**

**Function :** mV Measurement

**Performing standard curve by Document Process Calibrator at pH (4,7)(7,10)**

Unit Under Calibration	Nominal Value	Standard Voltage Input	Actual Reading		Uncertainty of Measurement { ±mV }	Coverage factor k
	pH	mV	mV	pH		
pH Meter S/N.: JC02728	4.00	177.48	177	4.01	0.58	2.00
	7.00	0.00	0	7.00	0.58	2.00
	7.00	0.00	0	7.00	0.58	2.00
	10.00	-177.48	-177	10.01	0.58	2.00

เอกสารไม่ควบคุม



Cert.No.: 25CH881

Page.: 3 of 3

**Calibration Results****Function : pH Measurement****Performing three buffers standard curve by using buffer nominal pH (4,7)(7,10)**

Unit Under Calibration	Standard pH Buffer Solution	Actual pH Reading	Actual mV Reading (mV)	Uncertainty of pH Measurement ( $\pm$ )	Coverage factor $k$
pH Electrode S/N.: 2403D4SIA605377	4.007	4.01	171	0.0079	2.00
	7.000	6.99	-3	0.0095	2.00
	7.000	7.00	-3	0.0092	2.00
	10.010	10.00	-174	0.0095	2.00

**Function : Temperature Measurement****(\*) Without adjustment**

This equipment was connected with Temperature Probe:

- Model :

-

- Serial No. :

240904SIA605377

Dimension of probe

- Length :

110 mm

- Diameter :

12 mm.

- Immersion Depth :

100 mm.

Calibration Point ( $^{\circ}\text{C}$ )	Standard Temperature ( $^{\circ}\text{C}$ )	UUC* Reading ( $^{\circ}\text{C}$ )	Error ( $^{\circ}\text{C}$ )	Uncertainty of measurement ( $\pm$ $^{\circ}\text{C}$ )	Coverage factor $k$
15.0	15.002	14.9	-0.102	0.13	2.00
30.0	30.002	30.0	-0.002	0.13	2.00
45.0	45.003	44.9	-0.103	0.13	2.00

**Remark** - UUC\* = Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor  $k$ , providing a level of confidence of approximately 95 %.

-o0o-

เอกสารไม่ควบคุม

## List of Instrument Certificates for Environmental Quality Analysis

No.	Instrument/Equipment	Parameter	Manufacturer	Model/Serial No.	Calibrator	Certification No.	Date of Calibration	Due date of Calibration*
1	Incubator	ESCHERICHIA COLI	Binder	KB400 / 20220000022479	National food institute ministry of Industry	2503682 004 01	1/7/2025	30/6/2026

**Due Date of Calibration\*** : Based on the annual calibration plan. At least 1 time per year.

## Calibration Certificate

**Certificate No.:** 2503682-004-01  
**Client name:** UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.  
**Address:** 3 Soi Udomsuk 41, Sukhumvit Road,  
Bangchack, Prakhnong, Bangkok 10260

Page 1 of 3

**Equipment:** CHAMBER (Incubator)

**Manufacturer:** BINDER

**Model:** KB 400

**Serial No.:** 20220000022479

**ID No.:** UAE.MIC.028/2566


**Order No.:** 2503682

**Operation No.:** 2503682-004

**Date of Receipt:** 1 July 2025

**Date of Calibration:** 1 July 2025

**Calibrated by** Mr.Pheraphat Tuanjit  
Scientist

**Approved by**   
( Miss Preeyaporn Jaengkarnkit )  
Vice President, Department of Laboratory Services  
Responsible for the Technical Management Team

**Date of Issue:** 3 July 2025

The uncertainties are for a confidence probability of approximately 95 %.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the National Food Institute.

F-CS-009 Revision: 01 Date: 20-04-65





## Calibration Report

**Certificate No.:** 2503682-004-01  
**Equipment:** CHAMBER (Incubator)  
Model: KB 400 Serial No.: 20220000022479  
Resolution: 0.1 °C ID No.: UAE.MIC.028/2566  
Manufacturer: BINDER  
**Date of Calibration:** 1 July 2025

Page 2 of 3

**Location:** Microbiology Laboratory, UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.  
**Environment Condition:** Ambient Temperature ( 21 ± 1 ) °C  
Relative Humidity ( 55 ± 10 ) %  
Line Voltage ( 230 ± 5 ) Volt

### Condition of this results of Calibration:

- This instrument was calibrated by insert 13 standard thermometer into its chamber and calibration according to W-TE-014 Based on TLAS G-20-1/02-08 (E): Guidelines for Calibration and Checks of Temperature Controlled Enclosures.  
- The temperature scale used was based on ITS - 90.  
- All data show below were final values and the initial data may be obtained upon request.

### 2. Reference Standard Instrument :

Instrument	Model	Serial No./ID No.	Certificate No.	Due Date	Through
Digital Thermometer with sensor	34972A	MY59003377	2501168-001-01	13 January 2026	NATIONAL FOOD INSTITUTE
	RTD	CH#101-203 / RTD#101-203			

- This certificate is traceable to International System of Units (SI Units).
- This certificate was certified only for the instrument we calibrated.
- This result of calibration was found accurate as shown on date and place of calibration only.
- Condition of Calibrated item : Good

### UUC Description :

Time of Record 1 Hour 9 Minute At 35.0 °C  
Fresh air Damper - Open Position -  
X Close Fan 100%  
- Not Available

7. Result of Calibration : ☒ Without adjustment ☐ After adjustment

## Calibration Report

**Certificate No.:** 2503682-004-01  
**Equipment:** CHAMBER (Incubator)  
**Model:** KB 400 **Serial No.:** 20220000022479  
**Resolution:** 0.1 °C **ID No.:** UAE.MIC.028/2566  
**Manufacturer:** BINDER

**Date of Calibration:** 1 July 2025

Page 3 of 3

**Calibration point:** 35.0 °C

**Calibration result:**

Calibration Condition	Temperature (°C)	Relative Humidity (%)	Line Voltage (Volt)
MIN	20.1	45	225.0
MAX	22.0	65	235.0

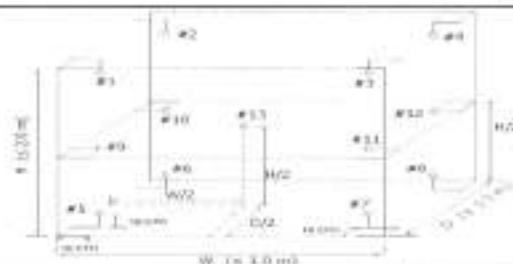


Table 1 : Reporting of Temperature

Calibration point (°C)	Measured Temperature (°C) @ Sensor No. (Sensor No.13 is REF)													Uncertainty ± (°C)
	# 1	# 2	# 3	# 4	# 5	# 6	# 7	# 8	# 9	# 10	# 11	# 12	# 13	
35.0	35.19	35.03	34.83	35.21	34.96	34.94	34.84	34.84	35.06	34.94	35.15	34.79	34.92	0.27

Table 2 : Reporting of Characterization Result

UUC* Setting (°C)	UUC* Reading (°C)			Temperature Stability ± (°C)	Temperature Uniformity (°C)	Overall Variation (°C)
	MIN	MAX	Average			
34.8	34.8	34.8	34.8	0.040	0.29	0.50

**Note** The quoted uncertainty include " Stability " and " Loading effect (20% of Temp Uniformity) "

UUC\* = Unit Under Calibration

Stability = One-half of the greatest maximum difference of measured temperatures at any one sensors, for at least half an hour after reaching steady state.

Uniformity = The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time.

Overall Variation = The difference of the maximum and minimum measured temperatures throughout observation time.

The report uncertainty of measurement was based on standard uncertainty multiplied by coverage factor  $k=2$ , providing a level of confidence of approximately 95 %.

----- End -----

3 July 2025

เอกสารไม่ควบคุม



## List of Instrument Certificates for Environmental Quality Analysis

No.	Instrument/Equipment	Parameter	Manufacturer	Model/Serial No.	Calibrator	Certification No.	Date of Calibration	Due date of Calibration*
1	Incubator	LEGIONELLA SP.	Memmert	IPP260 / V616.0066	National Food Institute, Ministry of Industry, Thailand	2502229-002-01	19/3/2025	18/3/2026

**Due Date of Calibration\*** : Based on the annual calibration plan. At least 1 time per year.

## Calibration Certificate

**Certificate No.:** 2502229-002-01  
**Client name:** UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.  
**Address:** 3 Soi Udomsuk 41, Sukhumvit Road,  
Bangchack, Prakhnong, Bangkok 10260

Page 1 of 3

**Equipment:** CHAMBER (Incubator)  
**Manufacturer:** MEMMERT  
**Model:** IPP260  
**Serial No.:** V616.0066  
**ID No.:** UAE.MIC.032/2559  
**Order No.:** 2502229  
**Operation No.:** 2502229-002  
**Date of Receipt:** 19 March 2025  
**Date of Calibration:** 19 March 2025

**Calibrated by** Mr.Yothin Charoensuk  
Scientist

**Approved by**

( Mr.Pheraphat Tuanjit )  
Manager, Division of Calibration Laboratory  
Responsible for the Technical Management Team

**Date of Issue:** 25 March 2025

The uncertainties are for a confidence probability of approximately 95 %.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the National Food Institute.

F-CS-009 Revision: 01 Date: 20-04-65

เอกสารไม่ควบคุม







## Calibration Report

**Certificate No.:** 2502229-002-01  
**Equipment:** CHAMBER (Incubator)  
**Model:** IPP260 **Serial No.:** V616.0066  
**Resolution:** 0.1 °C **ID No.:** UAE.MIC.032/2559  
**Manufacturer:** MEMMERT


**Date of Calibration:** 19 March 2025

Page 3 of 3

**Calibration point:** 25.0 and 36.0 °C

**Calibration result:**

Calibration Condition	Temperature (°C)	Relative Humidity (%)	Line Voltage (Volt)
MIN	21.3	58	220.0
MAX	22.0	60	225.0

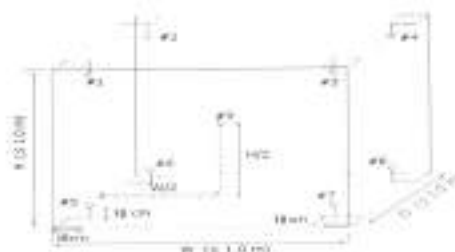

**Table 1 : Reporting of Temperature**

Calibration point (°C)	Measured Temperature (°C) @ Sensor No. (Sensor No.9 is REF)									Uncertainty ± (°C)
	# 1	# 2	# 3	# 4	# 5	# 6	# 7	# 8	# 9	
25.0	25.19	25.16	25.22	25.17	24.85	24.91	24.78	24.85	24.97	0.29
36.0	34.57	34.74	35.13	35.29	36.32	36.16	36.20	36.34	35.73	0.63

**Table 2 : Reporting of Characterization Result**

UUC* Setting (°C)	UUC* Reading (°C)			Stability ± (°C)	Uniformity (°C)	Overall Variation (°C)
	MIN	MAX	Average			
25.0	24.9	25.0	25.0	0.088	0.25	0.61
36.0	35.9	36.0	36.0	0.44	1.2	2.3

**Note** The quoted uncertainty include " Stability " and " Loading effect (20% of Temp Uniformity) "

UUC\* = Unit Under Calibration

Stability = One-half of the greatest maximum difference of measured temperatures at any one sensors, for at least half an hour after reaching steady state.

Uniformity = The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time.

Overall Variation = The difference of the maximum and minimum measured temperatures throughout observation time.

The report uncertainty of measurement was based on standard uncertainty multiplied by coverage factor  $k=2$ , providing a level of confidence of approximately 95 %.

----- End -----

