

ภาคผนวก จ
เอกสารสอบเทียบเครื่องมือ

List of Instruments Certification for Water Quality Analysis

No.	Instrument/Equipment	Parameter	Manufacturer	Model/Serial No.	Calibrator	Certification No.	Date of Calibration	Due date of Calibration	Remark
Water									
1	pH Meter	pH	Horiba	LAQUA-PH210 HA0D0081	Technology Promotion Association (Thailand-Japan)	25CH736	23 Jun 25	22 Jun 26	-
2	pH Meter	pH	Horiba	LAQUA-PH210 HA1G0008	Technology Promotion Association (Thailand-Japan)	25CH1022	28 Aug 25	27 Aug 26	-

รายการใบรับรองสอบเทียบ/ทวนสอบ เครื่องมือหลักประจำห้องปฏิบัติการวิเคราะห์ สำหรับวิเคราะห์คุณภาพสิ่งแวดล้อม

No.	Instrument/Equipment	Parameter	Manufacturer	Model/Serial No.	Calibrator	Certification No.	Date of Calibration	Due date of Calibration*	Remark
เครื่องมือหลักประจำห้องปฏิบัติการวิเคราะห์คุณภาพน้ำ									
1	pH Meter	pH	Horiba	LAQUA-PH210 / HA1M0043	Technology Promotion Association (Thailand-Japan)	25CH263	28 Feb 25	27 Feb 26	-
2	pH Meter	pH	Horiba	LAQUA-PH210 / HA0C0025	Technology Promotion Association (Thailand-Japan)	25CH261	26 Feb 25	25 Feb 26	-
3	Analytical Balance	Total Suspended Solids	Mettler-Toledo	XSR205DU / C009071872	National Food Institute, Ministry of Industry, Thailand	2502226-001-01	20 Mar 25	19 Mar 26	-
4	Analytical Balance	Total Dissolved Solids	Memmert	XSR205DU / C210685394	Technology Promotion Association (Thailand-Japan)	2502226-002-01	20 Mar 25	19 Mar 26	-
5	Analytical Balance	Oil & Grease, Fat	Mettler-Toledo	AB204-S / FACT / 1129361010	United Analyst and Engineering Consultant Co.; Ltd.	250422 1 BL 002 25	23 Apr 25	22 Apr 26	-
6	DO Meter	BOD	YSI	5100 / 11B 101863	Technology Promotion Association (Thailand-Japan)	25TW29	18 Feb 25	17 Feb 26	-
7	BOD Incubator	BOD	Arco	UC4-1320 / -	Technology Promotion Association (Thailand-Japan)	25TM578	19 Mar 25	18 Mar 26	-
8	BOD Incubator	BOD	Arco	UC4-1320 / -	Technology Promotion Association (Thailand-Japan)	25TM1003	8 Jul 25	7 Jul 26	-
9	Digestor Unit	Nitrogen (TKN)	Foss Tecator	2520 Auto / 91794469	National Food Institute, Ministry of Industry, Thailand	2501440-001-01	27 Jan 25	26 Jan 26	-
10	UV-VIS Spectrophotometer	Nitrate	Hitachi	U-2900 / 21E22-009	DQE Services Co.,Ltd.	SP25-001	3 Jan 25	2 Jan 26	-
11	UV-VIS Spectrophotometer	Ammonia	Hitachi	U-5100 / 23A4-008	DQE Services Co.,Ltd.	SP25-024	17 Jun 25	16 Jun 26	-
12	Cooled Incubator	Fecal Coliform Bacteria Total Coliform Bacteria , E.coli	Binder	KB400 / WTB20200000015535	National Food Institute, Ministry of Industry, Thailand	2502229-006-01	19 Mar 25	18 Mar 26	-
13	Incubator	P.aeruginosa	Memmert	IF75 / D317.0305	National Food Institute, Ministry of Industry, Thailand	2502229-004-01	20 Mar 25	19 Mar 26	-
14	Incubator	S. aureus	Memmert	IPP 260 / V615.0187	National Food Institute, Ministry of Industry, Thailand	2502229-001-01	19 Mar 25	18 Mar 26	-
15	Cyanuric Acid Photometer	Cyanuric Acid	Hanna Instrument Inc.,Romania	HI97722C / 905060O58111	Hanna Instruments (Thailand) Ltd.	HIT-2513-0437	24 Mar 25	23 Mar 26	-

Due Date of Calibration* : Based on the annual calibration plan. At least 1 time per year.



Certificate of Calibration

Cert.No.: 25CH736
Page.: 1 of 3

Equipment : pH Meter
Manufacturer : Horiba
Model : LAQUA-PH210
Serial No. : HA0D0081
ID No. : UAE.EFM.074/2564(EFM.pH.07/64)
Condition As-Received: Used Item
Received Date : 18 June 2025
Calibration Date : 23 June 2025
Reference : 2506-0591WSC-3
Submitted by : United Analyst and Engineering Consultant Co.,Ltd.
3 Soi Udomsuk 41, Sukhumvit Road, Bangchak,
Phrakhanong, Bangkok 10260
Ambient Temperature : (25 ± 2.5) °C
Relative Humidity : (50 ± 15) %
Calibration Procedure : In - house method :
- CP-CH5 by direct measurement with DC voltage
standard and direct measurement with
certified reference material (CRM)
- CP-CH8 by comparison with temperature standard

Calibrated by :

Approved by :

Approved Signatory

()
()
(✓)

Issue Date :

24 June 2025

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

เอกสารไม่ควบคุม

Condition of this calibration result

1. Reference Standard Instrument

Instrument	Serial No.	ID No.	Cert. No.	Due Date
1) Document Process Calibrator	54030049	130RC116	24E2759	25 Aug 2025
2) Ref. Standard Thermometer	4982054	110RC044	24I757	14 July 2025

- This measurement result is traceable to SI through Technology Promotion Association (Thailand - Japan)

2. Certified Reference Materials

:The measurement results are traceable to SI through Hach Lenge GmbH Ltd.,
Deutsche Akkreditierungsstelle, Accredited No.D-RM-15184-01-00
:The measurement results are traceable to SI through CPA chem Ltd.,
ANSI-ASQ National Accreditation Board, Accredited No. AR-1835

Buffer Solution	Manufacturer	Lot No.	Exp. date
pH 4.007	CPA chem	1066665	18 Jan 2027
pH 7.000	Hach Lenge GmbH	C03232	02 Dec 2026
pH 10.010	CPA chem	1066669	18 Jan 2026

3. This certificate is valid only to the item calibrated on date and place of calibration.

Calibration Results

Function : mV Measurement

Performing standard curve by Document Process Calibrator at pH (4,7)(7,10)

Unit Under Calibration	Nominal Value	Standard Voltage Input	Actual Reading		Uncertainty of Measurement (±mV)	Coverage factor k
			mV	pH		
pH Meter S/N.: HA0D0081	4.00	177.48	177.4	4.01	0.058	2.00
	7.00	0.00	0.0	6.98	0.058	2.00
	7.00	0.00	0.0	6.98	0.058	2.00
	10.00	-177.48	-177.4	10.01	0.058	2.00

Certificate of Calibration

Cert.No.: 25CH1022
Page.: 1 of 3

Equipment : pH Meter
Manufacturer : Horiba
Model : LAQUA-PH210
Serial No. : HA1G0008
ID No. : UAE.EFM.201/2564(EFM.pH.09/64)
Condition As-Received: Used Item
Received Date : 27 August 2025
Calibration Date : 28 August 2025
Reference : 2808-0874WSC-1
Submitted by : United Analyst and Engineering Consultant Co.,Ltd.
3 Soi Udomsuk 41, Sukhumvit Road, Bangchak,
Phrakhanong, Bangkok 10260
Ambient Temperature : (25 ± 2.5) °C
Relative Humidity : (50 ± 15) %
Calibration Procedure : In - house method :
- CP-CH5 by direct measurement with DC voltage
standard and direct measurement with
certified reference material (CRM)
- CP-CH8 by comparison with temperature standard

Calibrated by :

Approved by :

Approved Signatory

()
()
(✓)

Issue Date :

29 August 2025

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services

เอกสารไม่ควบคุม



Cert.No.: 25CH736
Page.: 3 of 3

Calibration Results

Function : pH Measurement

Performing three buffers standard curve by using buffer nominal pH (4,7)(7,10)

Unit Under Calibration	Standard pH Buffer Solution	Actual pH Reading	Actual mV Reading (mV)	Uncertainty of pH Measurement (±)	Coverage factor k
pH Electrode S/N.: -	4.007	4.01	176.5	0.0079	2.00
	7.000	6.98	0.8	0.0085	2.00
	7.000	7.00	-0.7	0.0095	2.00
	10.010	10.01	-172.7	0.0092	2.00

Function : Temperature Measurement

(*) Without adjustment

This equipment was connected with Temperature Probe;

- Model : -

- Serial No. : -

Dimension of probe

- Length : 103 mm.

- Diameter : 16 mm.

- Immersion Depth : 90 mm.

Calibration Point (°C)	Standard Temperature (°C)	UUC* Reading (°C)	Error (°C)	Uncertainty of measurement (± °C)	Coverage factor k
15.0	15.000	15.0	0.000	0.13	2.00
30.0	30.000	30.0	0.000	0.13	2.00
45.0	45.003	45.0	-0.003	0.13	2.00

Remark - UUC* = Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k , providing a level of confidence of approximately 95 %.

-o0o-

เอกสารไม่ควบคุม



Cert.No.: 25CH1022
Page: 2 of 3

Condition of this calibration result

1. Reference Standard Instrument

Instrument	Serial No.	ID No.	Cert. No.	Due Date
1) Document Process Calibrator	58440003	130RC120	24E3731	25 Nov 2025
2) Ref. Standard Thermometer	4982054	110RC044	25I708	03 July 2026

- This measurement result is traceable to SI through Technology Promotion Association (Thailand - Japan)

2. Certified Reference Materials :The measurement results are traceable to SI through Hach Lenge GmbH Ltd.,
Deutsche Akkreditierungsstelle, Accredited No.D-RM-15184-01-00
:The measurement results are traceable to SI through CPA chem Ltd.,
ANSI-ASQ National Accreditation Board, Accredited No. AR-1835

Buffer Solution	Manufacturer	Lot No.	Exp. date
pH 4.007	CPA chem	1114384	12 June 2027
pH 6.999	Hach Lenge GmbH	C03273	13 May 2027
pH 10.010	CPA chem	1114385	08 June 2026

3. This certificate is valid only to the item calibrated on date and place of calibration.

Calibration Results

Function : mV Measurement

Performing standard curve by Document Process Calibrator at pH (4,7)(7,10)

Unit Under Calibration	Nominal Value	Standard Voltage Input	Actual Reading		Uncertainty of Measurement	Coverage factor
	pH	mV	mV	pH	($\pm$ mV)	k
pH Meter S/N.: HA1G0008	4.00	177.48	177.6	4.01	0.058	2.00
	7.00	0.00	0.1	7.02	0.058	2.00
	7.00	0.00	0.1	7.02	0.058	2.00
	10.00	-177.48	-177.4	10.01	0.058	2.00



Cert.No.: 25CH1022
Page: 3 of 3

Calibration Results

Function : pH Measurement

Performing three buffers standard curve by using buffer nominal pH (4,7)(7,10)

Unit Under Calibration	Standard pH Buffer Solution	Actual pH Reading	Actual mV Reading (mV)	Uncertainty of pH Measurement ($\pm$)	Coverage factor k
pH Electrode S/N.: Q9BF0102	4.007	4.00	181.1	0.0079	2.00
	6.999	6.98	7.1	0.0095	2.00
	6.999	7.00	8.0	0.0096	2.00
	10.010	10.01	-162.8	0.0092	2.00

Function : Temperature Measurement

(*) Without adjustment

This equipment was connected with Temperature Probe;

- Model : 9652-10
- Serial No. : Q9BF0102
Dimension of probe
- Length : 110 mm.
- Diameter : 16 mm.
- Immersion Depth : 90 mm.

Calibration Point (°C)	Standard Temperature (°C)	UUC* Reading (°C)	Error (°C)	Uncertainty of measurement ($\pm$ °C)	Coverage factor k
15.0	15.001	15.0	-0.001	0.13	2.00
30.0	29.998	30.0	0.002	0.13	2.00
45.0	45.002	45.0	-0.002	0.13	2.00

Remark : - UUC* = Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k, providing a level of confidence of approximately 95 %.

-o0o-

เอกสารไม่ควบคุม

เอกสารไม่ควบคุม



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL.0-2717-3000-29 FAX.0-2719-9484



Certificate of Calibration

Cert.No.: 25CH263
Page: 1 of 3

Equipment : pH Meter
Manufacturer : Horiba
Model : LAQUA-PH210
Serial No. : HA1M0043
ID No. : UAE.EFM.013/2565(EFM.pH.03/65)
Condition As-Received: Used Item
Received Date : 25 February 2025
Calibration Date : 26 to 28 February 2025
Reference : 2502-0783WSC-3
Submitted by : United Analyst and Engineering Consultant Co.,Ltd.
3 Soi Udomsuk 41, Sukhumvit Road,
Bangchak, Phrakhanong, Bangkok 10260

Ambient Temperature : (25 $\pm$ 2.5) °C
Relative Humidity : (50 $\pm$ 15) %
Calibration Procedure : In - house method :
- CP-CH5 by direct measurement with DC voltage standard and direct measurement with certified reference material (CRM)
- CP-CH8 by comparison with temperature standard

Calibrated by :

Approved by :

()
()
(✓)

Issue Date : 28 February 2025

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

เอกสารไม่ควบคุม



Cert.No.: 25CH263
Page: 2 of 3

Condition of this calibration result

1. Reference Standard Instrument

Instrument	Serial No.	ID No.	Cert. No.	Due Date
1)Document Process Calibrator	54030049	130RC116	24E2759	25 Aug 2025
2)Ref. Standard Thermometer	4982054	110RC044	24I757	14 July 2025

- This Certification is traceable to SI Through Technology Promotion Association (Thailand - Japan)

2. Certified Reference Materials :The measurement results are traceable to SI through Hach Lenge GmbH Ltd.,
Deutsche Akkreditierungsstelle, Accredited No.D-RM-15184-01-00
: The measurement results are traceable to SI through CPA chem Ltd.,
ANSI-ASQ National Accreditation Board, Accredited No. AR-1835

Buffer Solution	Manufacturer	Lot No.	Exp. date
pH 4.007	CPA chem	1066665	18 Jan 2027
pH 6.999	Hach Lenge GmbH	C03220	29 Oct 2026
pH 10.010	CPA chem	1066669	18 Jan 2026

3. This certificate is valid only to the item calibrated on date and place of calibration.

Calibration Results

Function : mV Measurement

Performing standard curve by Document Process Calibrator at pH (4,7)(7,10)

Unit Under Calibration	Nominal Value	Standard Voltage Input	Actual Reading		Uncertainty of Measurement	Coverage factor
	pH	mV	mV	pH	($\pm$ mV)	k
pH Meter S/N.: HA1M0043	4.00	177.48	177.4	4.01	0.058	2.00
	7.00	0.00	-0.1	7.00	0.058	2.00
	7.00	0.00	-0.1	7.00	0.058	2.00
	10.00	-177.48	-177.6	10.01	0.058	2.00

เอกสารไม่ควบคุม



Cert.No.: 25CH263
Page.: 3 of 3

Calibration Results

Function : pH Measurement

Performing three buffers standard curve by using buffer nominal pH (4,7)(7,10)

Unit Under Calibration	Standard pH Buffer Solution	Actual pH Reading	Actual mV Reading (mV)	Uncertainty of pH Measurement (±)	Coverage factor <i>k</i>
pH Electrode S/N.: 992H0385	4.007	4.01	147.9	0.0085	2.05
	6.999	7.00	-24.3	0.0092	2.00
	6.999	7.01	-24.4	0.0085	2.00
	10.010	10.01	-197.8	0.0092	2.00

Function : Temperature Measurement

(*) Without adjustment

This equipment was connected with Temperature Probe;

- Model : 9652

- Serial No. : 992H0385

Dimension of probe

- Length : 110 mm.

- Diameter : 16 mm.

- Immersion Depth : 80 mm.

Calibration Point (°C)	Standard Temperature (°C)	UUC* Reading (°C)	Error (°C)	Uncertainty of measurement (± °C)	Coverage factor <i>k</i>
15.0	15.003	15.0	-0.003	0.13	2.00
30.0	30.004	30.0	-0.004	0.13	2.00
45.0	45.002	45.0	-0.002	0.13	2.00

Remark - UUC* = Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

เอกสารไม่ควบคุม



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL.0-2717-3000-29 FAX.0-2719-9484



Certificate of Calibration

Cert.No.: 25CH261
Page.: 1 of 3

Equipment : pH Meter
Manufacturer : Horiba
Model : LAQUA-PH210
Serial No. : HA0C0025
ID No. : UAE.EFM.117/2563(EFM.pH.07/63)
Condition As-Received: Used Item
Received Date : 25 February 2025
Calibration Date : 26 to 28 February 2025
Reference : 2502-0783WSC-1
Submitted by : United Analyst and Engineering Consultant Co.,Ltd.
3 Soi Udomsuk 41, Sukhumvit Road,
Bangchak, Phrakhanong, Bangkok 10260

Ambient Temperature : (25 ± 2.5) °C
Relative Humidity : (50 ± 15) %
Calibration Procedure : In - house method :
- CP-CH5 by direct measurement with DC voltage standard and direct measurement with certified reference material (CRM)
- CP-CH8 by comparison with temperature standard

Calibrated by :

Approved by :

Approved Signatory

()

()

(✓)

Issue Date :

28 February 2025

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written Approval of the head of Corporate Services 3: Equipment Calibration and Testing Services.

เอกสารไม่ควบคุม



Cert.No.: 25CH261
Page.: 2 of 3

Condition of this calibration result

1. Reference Standard Instrument

Instrument	Serial No.	ID No.	Cert. No.	Due Date
1)Document Process Calibrator	54030049	130RC116	24E2759	25 Aug 2025
2)Ref. Standard Thermometer	4982054	110RC044	24I757	14 July 2025

- This Certification is traceable to SI Through Technology Promotion Association (Thailand - Japan)

2. Certified Reference Materials :The measurement results are traceable to SI through Hach Lenge GmbH Ltd.,

Deutsche Akkreditierungsstelle, Accredited No.D-RM-15184-01-00

: The measurement results are traceable to SI through CPA chem Ltd.,

ANSI-ASQ National Accreditation Board, Accredited No. AR-1835

Buffer Solution	Manufacturer	Lot No.	Exp. date
pH 4.007	CPA chem	1066665	18 Jan 2027
pH 6.999	Hach Lenge GmbH	C03220	29 Oct 2026
pH 10.010	CPA chem	1066669	18 Jan 2026

3. This certificate is valid only to the item calibrated on date and place of calibration.

Calibration Results

Function : mV Measurement

Performing standard curve by Document Process Calibrator at pH (4,7)(7,10)

Unit Under Calibration	Nominal Value	Standard Voltage Input	Actual Reading		Uncertainty of Measurement (± mV)	Coverage factor <i>k</i>
	pH	mV	mV	pH		
pH Meter S/N.: HA0C0025	4.00	177.48	177.5	4.01	0.058	2.00
	7.00	0.00	0.0	7.02	0.058	2.00
	7.00	0.00	0.0	7.02	0.058	2.00
	10.00	-177.48	-177.5	10.01	0.058	2.00

Calibration Results

Function : pH Measurement

Performing three buffers standard curve by using buffer nominal pH (4,7)(7,10)

Unit Under Calibration	Standard pH Buffer Solution	Actual pH Reading	Actual mV Reading (mV)	Uncertainty of pH Measurement (±)	Coverage factor <i>k</i>
pH Electrode S/N.: Q9AG0214	4.007	4.01	178.4	0.0071	2.00
	6.999	7.00	4.1	0.0092	2.00
	6.999	7.00	3.0	0.0095	2.00
	10.010	10.01	-169.8	0.0092	2.00

Function : Temperature Measurement

(*) Without adjustment

This equipment was connected with Temperature Probe;

- Model : 9652-10D

- Serial No. : Q9AG0214

Dimension of probe

- Length : 110 mm.

- Diameter : 16 mm.

- Immersion Depth : 80 mm.

Calibration Point (°C)	Standard Temperature (°C)	UUC* Reading (°C)	Error (°C)	Uncertainty of measurement (± °C)	Coverage factor <i>k</i>
15.0	15.002	15.0	-0.002	0.13	2.00
30.0	30.003	30.0	-0.003	0.13	2.00
45.0	45.002	44.9	-0.102	0.13	2.00

Remark - UUC* = Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

เอกสารไม่ควบคุม


เอกสารไม่ควบคุม

Calibration Certificate

Certificate No.: 2502226-001-01
Client name: UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.
Address: 3 Soi Udomsuk 41, Sukhumvit Road,
Bangchack, Prakhonong, Bangkok 10260

Page 1 of 4

Equipment: Electronic Balance
Manufacturer: METTLER TOLEDO
Model: XSR205DU
Serial No.: C009071872
ID No.: UAE.WAO.012/2563
Order No.: 2502226
Operation No.: 2502226-001
Date of Receipt: 19 March 2025
Date of Calibration: 20 March 2025

Calibrated by  **Approved by** 
Scientist Manager, Division of Calibration Laboratory
Responsible for the Technical Management Team
Date of Issue: 25 March 2025

The uncertainties are for a confidence probability of approximately 95%

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the National Food Institute.

FCS-009 Revision: 01 Date: 20-04-65

2009 บอยสภพพ. 36 อรุณ อรุณโรด, บาง ย์ ราช สหราช, บาง พรี ดิสท, กรุงเทพฯ 10700, Thailand
Tel: +66(0) 2422 8688 Fax: +66(0) 2422 8545



Calibration Report

Certificate No.: 2502226-001-01
Equipment: Electronic Balance
Model: XSR205DU
Serial No.: C009071872
Capacity: 82 g / 220 g
Manufacturer: METTLER TOLEDO
Resolution: 0.00001 g / 0.0001 g
ID No.: UAE.WAO.012/2563

Page 2 of 4

Date of Calibration: 20 March 2025
Environment Condition: Ambient Temperature: 21.2 ± 0.6 °C Relative Humidity: 48 ± 3.5 %
Place of Calibration: 208 Balance Room, UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.
Condition of Equipment: Good Condition
Condition of This Results of Calibration:
1. Calibration Method: NFI Method W-MA-001 In-House Method based on UKAS Lab 14 : 2019
2. Reference Standards:
Reference Standard **Model** **Serial No.** **Calibrated By** **Certificate No.** **Due Date**
Standard Weight Class E2 1mg to 200g 8505567572 TCS M24041005 19 April 2025
Instrument **Model** **Serial No.** **Calibrated By** **Certificate No.** **Due Date**
Thermo-Hygro Meter 608-H1 NFI.BTH 017/23 Quality Reborn QR25-0542 10 February 2026
3. This certification is traceable to SI UNIT
4. This certificate was certified only for the instrument we calibrated.
5. This result of calibration was found accurate as shown on date and place of calibration only.

Calibration Results:


1. Repeatability of Reading:

Nominal Value (g)	Standard Deviation of Reading (g)
40	0.0000052
80	0.0000042
100	0.0000000
200	0.0000000

2. Off-Center Error:

A mass of 100 g was placed and moved to various position on pan.

The balance reading obtained is given in the table.



1	2	3	4	5	6	(Maximum Difference)
(g)	(g)	(g)	(g)	(g)	(g)	(g)
100.0001	100.0001	100.0001	100.0001	100.0001	100.0002	0.0001

FCS-012 Revision: 01 Date: 20-04-65

2009 บอยสภพพ. 36 อรุณ อรุณโรด, บาง ย์ ราช สหราช, บาง พรี ดิสท, กรุงเทพฯ 10700, Thailand
Tel: +66(0) 2422 8688 Fax: +66(0) 2422 8545



Calibration Report

Certificate No.: 2502226-001-01
Equipment: Electronic Balance
Model: XSR205DU
Serial No.: C009071872
Capacity: 82 g / 220 g
Manufacturer: METTLER TOLEDO
Resolution: 0.00001 g / 0.0001 g
ID No.: UAE.WAO.012/2563

Page 3 of 4

Date of Calibration: 20 March 2025

Calibration Results: (Continued)

Calibration Range: 0-80 g

Calibration Adjustment: Internal Calibration

3. Departure from Nominal Value: (Range: 0 - 82 g ; Resolution: 0.00001 g)

Nominal Value (g)	Standard Value (g)	Average Reading (g)	Correction (g)	Uncertainty (± g)	Coverage Factor k
Unload	0.000000	0.000000	0.000000	0.0000089	2.00
0.001	0.001003	0.001000	0.000000	0.0000092	2.00
0.005	0.005002	0.005000	0.000000	0.0000094	2.00
0.01	0.010003	0.010000	0.000000	0.0000091	2.00
0.05	0.049996	0.050000	0.000000	0.0000098	2.00
0.1	0.100011	0.100000	0.000001	0.0000111	2.00
0.5	0.500016	0.500000	0.000002	0.000014	2.00
1	1.000003	1.000001	-0.000001	0.000016	2.00
2	2.000023	2.000005	-0.000003	0.000017	2.00
5	5.000015	5.000005	-0.000003	0.000021	2.00
10	10.000009	10.000005	-0.000004	0.000026	2.00
20	20.000030	20.000012	-0.000009	0.000037	2.00
30	30.000039	30.000012	-0.000008	0.000050	2.00
50	50.000028	50.000014	-0.000011	0.000068	2.00
80	80.000067	80.000020	-0.000013	0.00011	2.00

Calibration Report

Certificate No.: 2502226-001-01
Equipment: Electronic Balance
Model: XSR205DU
Serial No.: C009071872
Capacity: 82 g / 220 g
Manufacturer: METTLER TOLEDO
Resolution: 0.00001 g / 0.0001 g
ID No.: UAE.WAO.012/2563

Page 4 of 4

Date of Calibration: 20 March 2025

Calibration Results: (Continued)

Calibration Range: >80-200 g

Calibration Adjustment: Internal Calibration

3. Departure from Nominal Value: (Range: >80 - 200 g ; Resolution: 0.0001 g)

Nominal Value (g)	Standard Value (g)	Average Reading (g)	Correction (g)	Uncertainty (± g)	Coverage Factor k
90	90.000010	90.00002	-0.00001	0.000015	2.00
100	100.000006	100.00001	0.00000	0.000016	2.00
110	110.000007	110.00001	0.00000	0.000017	2.00
120	120.000009	120.00002	-0.00001	0.000018	2.00
130	130.000010	130.00002	-0.00001	0.000019	2.00
140	140.000013	140.00002	-0.00001	0.000019	2.00
150	150.000009	150.00002	-0.00001	0.000021	2.00
160	160.000010	160.00002	-0.00001	0.000022	2.00
170	170.000012	170.00002	-0.00001	0.000023	2.00
200	200.000013	200.00002	-0.00001	0.000028	2.00

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k, providing a level of confidence of approximately 95 %.

***** End *****

FCS-012 Revision: 01 Date: 20-04-65

2009 บอยสภพพ. 36 อรุณ อรุณโรด, บาง ย์ ราช สหราช, บาง พรี ดิสท, กรุงเทพฯ 10700, Thailand
Tel: +66(0) 2422 8688 Fax: +66(0) 2422 8545



FCS-012 Revision: 01 Date: 20-04-65

2009 บอยสภพพ. 36 อรุณ อรุณโรด, บาง ย์ ราช สหราช, บาง พรี ดิสท, กรุงเทพฯ 10700, Thailand
Tel: +66(0) 2422 8688 Fax: +66(0) 2422 8545



Calibration Certificate

Certificate No.: 2502226-002-01
Client name: UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.
Address: 3 Soi Udomsuk 41, Sukhumvit Road,
Bangchack, Prakhonong, Bangkok 10260

Page 1 of 4

Equipment: Electronic Balance
Manufacturer: METTLER TOLEDO
Model: XSR205DU
Serial No.: C210685394
ID No.: UAE.WAO.010/2565
Order No.: 2502226
Operation No.: 2502226-002
Date of Receipt: 19 March 2025
Date of Calibration: 20 March 2025

Calibrated by **Approved by**
Scientist
Manager, Division of Calibration Laboratory
Responsible for the Technical Management Team
Date of Issue: 25 March 2025

The uncertainties are for a confidence probability of approximately 95%

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full, except with the prior written approval of the National Food Institute.

F-CS-009 Revision: 01 Date: 20-04-65

2008 ปีที่ 35 ถนนสุขุมวิท แขวงคลองตัน เขตคลองเตย กรุงเทพมหานคร 10110
2008 Soi 35, Arun Amarin Road, Bang Yi Khan Subdistrict, Bang Phai District, Bangkok 10700, Thailand
Tel +66(0) 2422 8688 Fax +66(0) 2422 8545



Calibration Report

Certificate No.: 2502226-002-01
Equipment: Electronic Balance
Manufacturer: METTLER TOLEDO
Model: XSR205DU
Resolution: 0.00001 g / 0.0001 g
Serial No.: C210685394
ID No.: UAE.WAO.010/2565
Capacity: 82 g / 220 g

Page 2 of 4

Date of Calibration: 20 March 2025
Environment Condition: Ambient Temperature: 21.2 ± 0.6 °C Relative Humidity: 48 ± 3.5 %
Place of Calibration: 208 Balance Room, UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.
Condition of Equipment: Good Condition
Condition of This Results of Calibration:
1. Calibration Method: NFI Method W-MA-001 In-House Method based on UKAS Lab 14 : 2019
2. Reference Standards:
Reference Standard **Model** **Serial No.** **Calibrated By** **Certificate No.** **Due Date**
Standard Weight Class E2 1mg to 200g 8505567572 TCS M2401005 19 April 2025
Instrument **Model** **Serial No.** **Calibrated By** **Certificate No.** **Due Date**
Thermo-Hygro Meter 608-H1 NFI.BTH 017/23 Quality Reborn QR25-0542 10 February 2026
3. This certification is traceable to SI UNIT
4. This certificate was certified only for the instrument we calibrated.
5. This result of calibration was found accurate as shown on date and place of calibration only.

Calibration Results:


1. Repeatability of Reading:

Nominal Value (g)	Standard Deviation of Reading (g)
40	0.0000042
80	0.0000042
100	0.0000000
200	0.0000000

2. Off-Center Error:

A mass of 100 g was placed and moved to various position on pan.

The balance reading obtained is given in the table.



1 (g)	2 (g)	3 (g)	4 (g)	5 (g)	6 (g)	(Maximum Difference) (g)
100.0001	100.0001	100.0001	100.0001	100.0001	100.0001	0.0000

F-CS-012 Revision: 01 Date: 20-04-65

2008 ปีที่ 35 ถนนสุขุมวิท แขวงคลองตัน เขตคลองเตย กรุงเทพมหานคร 10110
2008 Soi 35, Arun Amarin Road, Bang Yi Khan Subdistrict, Bang Phai District, Bangkok 10700, Thailand
Tel +66(0) 2422 8688 Fax +66(0) 2422 8545



Calibration Report

Certificate No.: 2502226-002-01
Equipment: Electronic Balance
Manufacturer: METTLER TOLEDO
Model: XSR205DU
Resolution: 0.00001 g / 0.0001 g
Serial No.: C210685394
ID No.: UAE.WAO.010/2565
Capacity: 82 g / 220 g

Date of Calibration: 20 March 2025 **Page 3 of 4**

Calibration Results: (Continued)

Calibration Range: 0-80 g

Calibration Adjustment: Internal Calibration

3. Departure from Nominal Value: (Range: 0 - 82 g ; Resolution: 0.00001 g)

Nominal Value (g)	Standard Value (g)	Average Reading (g)	Correction (g)	Uncertainty (± g)	Coverage Factor k
Unloaded	0.000000	0.000000	0.000000	0.0000087	2.00
0.001	0.001003	0.001000	0.000000	0.0000090	2.00
0.005	0.005002	0.005001	-0.000001	0.0000092	2.00
0.01	0.010003	0.010002	-0.000002	0.0000089	2.00
0.05	0.049996	0.050001	-0.000001	0.0000096	2.00
0.1	0.100011	0.100002	-0.000009	0.0000111	2.00
0.5	0.500016	0.500004	-0.000012	0.000014	2.00
1	1.000003	1.000005	-0.000002	0.000016	2.00
2	2.000023	2.000006	-0.000017	0.000017	2.00
5	5.000015	5.000006	-0.000009	0.000020	2.00
10	10.000009	10.000005	-0.000004	0.000026	2.00
20	20.000030	20.000007	-0.000023	0.000037	2.00
30	30.000039	30.000009	-0.000030	0.000050	2.00
50	50.000028	50.000008	-0.000020	0.000068	2.00
80	80.000067	80.000013	-0.000054	0.000111	2.00

Page 3 of 4

F-CS-012 Revision: 01 Date: 20-04-65

2008 ปีที่ 35 ถนนสุขุมวิท แขวงคลองตัน เขตคลองเตย กรุงเทพมหานคร 10110
2008 Soi 35, Arun Amarin Road, Bang Yi Khan Subdistrict, Bang Phai District, Bangkok 10700, Thailand
Tel +66(0) 2422 8688 Fax +66(0) 2422 8545



Calibration Report

Certificate No.: 2502226-002-01
Equipment: Electronic Balance
Manufacturer: METTLER TOLEDO
Model: XSR205DU
Resolution: 0.00001 g / 0.0001 g
Serial No.: C210685394
ID No.: UAE.WAO.010/2565
Capacity: 82 g / 220 g

Date of Calibration: 20 March 2025 **Page 4 of 4**

Calibration Results: (Continued)

Calibration Range: >80-200 g

Calibration Adjustment: Internal Calibration

3. Departure from Nominal Value: (Range: >80 - 200 g ; Resolution: 0.00001 g)

Nominal Value (g)	Standard Value (g)	Average Reading (g)	Correction (g)	Uncertainty (± g)	Coverage Factor k
90	90.000010	90.000002	-0.000008	0.000015	2.00
100	100.000006	100.000001	-0.000005	0.000016	2.00
110	110.000007	110.000002	-0.000005	0.000017	2.00
120	120.000009	120.000002	-0.000007	0.000018	2.00
130	130.000010	130.000002	-0.000008	0.000019	2.00
140	140.000013	140.000002	-0.000011	0.000019	2.00
150	150.000009	150.000002	-0.000007	0.000021	2.00
160	160.000010	160.000002	-0.000008	0.000022	2.00
170	170.000012	170.000002	-0.000010	0.000023	2.00
200	200.000013	200.000002	-0.000011	0.000028	2.00

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k, providing a level of confidence of approximately 95 %.

***** End *****

F-CS-012 Revision: 01 Date: 20-04-65

2008 ปีที่ 35 ถนนสุขุมวิท แขวงคลองตัน เขตคลองเตย กรุงเทพมหานคร 10110
2008 Soi 35, Arun Amarin Road, Bang Yi Khan Subdistrict, Bang Phai District, Bangkok 10700, Thailand
Tel +66(0) 2422 8688 Fax +66(0) 2422 8545



Certificate of Calibration

Certificate No.: 250422-1-BL002-25

Code No.: BL002-25

Page: 1 of 3

Customer Name: United Analyst and Engineering Consultant Co., Ltd.
Address: 3 Soi Udom suk 41, Sukhumvit Rd., Bang Chak, Phar Khanong, Bangkok 10260

Equipment: Electronic Balance

Manufacturer: Mettler Toledo

Model: AB204-S/FACT

Serial No.: 1129361010

Asset No.: UAE.WAS.002/2552

Building: N/A

Floor: 1

Room: 107

Received Date: April 22, 2025

Date of Calibration: April 23, 2025

Calibration Conditions: Temperature 22.8 °C to 23.4 °C
Humidity 54.8 % to 68.9 %
Pressure 756.6 mmHg to 758.2 mmHg

Calibrated by:

Approved by:

Signature:

Issued Date: April 25, 2025

Note : 1) The Uncertainties are for a confidence probability of approximately 95%

2) This Certificate is valid only to the item calibrated on date and place of calibration.

3) This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the United Analyst and Engineering Consultant Co.,Ltd. (UAE)

เอกสารไม่ควบคุม

Certificate No.: 250422-1-BL002-25

Code No.: BL002-25

Page: 3 of 3

Equipment: Electronic Balance
Model: AB204-S/FACT
Serial No.: 1129361010
Max. Capacity: 220 g
Calibration Date: April 23, 2025

Manufacturer: Mettler Toledo
Readability: 0.0001 g
ID No.: UAE.WAS.002/2552

Calibration Result: (Continued)

Calibration Range: 0 - 200 g

Calibration Adjustment: Internal Calibration

3. Error of Indication from nominal or conventional mass value:

Nominal Value (g)	Reference Value (g)	Indication (g)	Correction (g)	Uncertainty (± mg)	Coverage Factor k
Unload	0.0000000	0.0000	0.0000	0.10	2.05
0.01	0.0100025	0.0099	0.0001	0.10	2.05
0.05	0.0500056	0.0500	0.0000	0.10	2.05
0.1	0.1000012	0.0999	0.0001	0.10	2.05
0.5	0.5000133	0.5000	0.0000	0.10	2.05
1	1.0000105	1.0000	0.0000	0.10	2.05
10	10.000010	10.0000	0.0000	0.11	2.04
40	40.000076	40.0000	0.0000	0.14	2.00
50	50.000056	50.0000	0.0001	0.13	2.00
80	80.000107	80.0000	0.0001	0.18	2.00
100	100.000109	99.9999	0.0002	0.17	2.00
120	120.00015	119.9999	0.0003	0.21	2.00
150	150.000165	149.9998	0.0003	0.24	2.00
160	160.000175	159.9997	0.0005	0.26	2.00
200	200.000129	199.9998	0.0004	0.30	2.00

4. Effect of Tare test:

Tare Load (g)	Test Load (g)	Indication (g)	Correction (g)
100	20.000041	19.9999	0.0001
	40.000076	39.9998	0.0002
	60.000066	59.9997	0.0003
	80.000107	79.9999	0.0002
	100.000168	100.0004	-0.0003

Remark:

The report uncertainty of measurement was based on standard uncertainty multiplied by coverage factor k, providing a level of confidence of approximately 95%.

o---o-End-o---o

เอกสารไม่ควบคุม

Certificate No.: 250422-1-BL002-25

Code No.: BL002-25

Page: 2 of 3

Equipment: Electronic Balance

Model: AB204-S/FACT

Serial No.: 1129361010

Max. Capacity: 220 g

Calibration Date: April 23, 2025

Condition As-Received: In Condition

Manufacturer: Mettler Toledo

Readability: 0.0001 g

ID No.: UAE.WAS.002/2552

Condition of Equipment:

Condition of This Result of Calibration:

1. Calibration Method: This instrument was calibrated by method UAE.CP.CAL.006 In-House Method based on UKAS Lab 14 : 2022

2. Reference Standards:

Reference Standard:	Model	Serial No.	Calibrated By	Certificate No.	Traceability	Due Date
Standard Weight Class E2 (OIML)	1 mg to 1 kg	8749109122	AMARC	25-009359	Mettler-Toledo	21-Jan-27
Standard Weight Class F1 (OIML)	1 mg to 200 g	11119512	AMARC	24-013840	Mettler-Toledo	04-Feb-26
Instrument	Model	Serial No.	Calibrated By	Certificate No.	Traceability	Due Date
Thermo-Hygro-Baro Meter	MHB-382SD	AK.46457	SUCCESS	SG-H-00997/67	Success Gateway	21-Nov-25
Thermo-Hygro-Baro Meter	MHB-382SD	AK.46457	TPA	25P795	TPA	25-Feb-26

3. This certification is traceable to SI Unit

4. This certification was certified only for the instrument we calibrated

5. This result of calibration was found accurate as shown on date and place of calibration only.

6. Through the reference standard laboratory of AMARC 25-009359 Calibration 0152

Calibration Result:


1. Repeatability of Reading:

Nominal Value (g)	Standard Deviation of Reading (g)
200*	0.000045

2. Eccentric or off-center loading

A mass of 100 g was placed and moved to various position on pan

The Balance reading obtained is given in the table.



1 (g)	2 (g)	3 (g)	4 (g)	5 (g)	Maximum Difference (g)
100.0000	99.9996	99.9997	100.0003	100.0005	0.0005

เอกสารไม่ควบคุม



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3 : EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000 FAX. 0-2719-9484

Certificate of Testing

Cert.No.: 25TW29

Page: 1 of 2

Equipment : DO Meter

Manufacturer : YSI

Model : 5100

Serial No. : 11B 101863

ID No. : UAE.WAO.004/2554

Received Date : 14 February 2025

Test Date : 17 February 2025

Reference : 2502-0473DSC-1

Submitted by : United Analyst and Engineering Consultant Co.,Ltd.
3 Soi Udomsuk 41, Sukhumvit Road, Bangkok, Phrakhanong, Bangkok 10260

Laboratory Condition :

Temperature (25 ± 5) °C

Humidity (50 ± 20) %

Test Procedure : In - house method : CP-CH9
by Comparison Technique with Azide Modification Method

Tested by :

Approved by :

Approved Signatory

()
()
(✓)

Issue Date :

18 February 2025

เอกสารไม่ควบคุม



Equipment : BOD Incubator
Condition As-Received : Used Item
Reference : 2503-04370C-2
Result of Calibration :- (*) Without Adjustment
Function of UUC* : Temperature Source
Fresh air setting : Close

Cert. No.: 25TM578
Page : 3 of 3

Calibration Point (°C)	UUC* Setting (°C)	UUC* Reading (°C)	Temperature stability (± °C)	Temperature uniformity (°C)	Overall Variation (°C)	Coverage Factor k
20.0	20.0	19.9	0.49	0.69	1.1	2

Calibration Point (°C)	Measured Temperature (°C)									Uncertainty (± °C)
	1	2	3	4	5	6	7	8	9 (ref.)	
20.0	20.025	19.753	20.063	19.839	20.103	20.086	20.152	20.211	19.804	0.69

Average* : The average of 30 values in each position.

Temperature stability : One-half of the greatest maximum difference of measured temperature at any one sensor.
Temperature uniformity : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.

Overall Variation : The Difference of the maximum and minimum measured temperatures throughout observation.

UUC* : Unit Under Calibration

Note : The reported uncertainty of measurement was included stability and excluded uniformity .

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k , providing a level of confidence of approximately 95 %.

-00o-

เอกสารไม่ควบคุม



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL.0-2717-3000-29 FAX.0-2719-9484



Certificate of Calibration

Cert. No.: 25TM1003
Page : 1 of 3

Equipment : BOD Incubator

Manufacturer : ARCO

Model : UC4-1320

Serial No. : -

ID No. : UAE.WAO.026/2566

Submitted by : United Analyst and Engineering Consultant Co.,Ltd.
3 Soi Udomsuk 41, Sukhumvit Road,
Bangchak, Phrakhanong,
Bangkok 10260

Location : Lab Floor 1

Received Order : 07 July 2025

Calibration Date : 08 July 2025

Ambient Temperature : (26 ± 10) °C

Relative Humidity : (50 ± 30) %

AC Line Voltage : (220 ± 22) V

Calibrated by :

Approved by :

Approved Signatory

() Chakrit Waewwanjua
() Suwit Imjai
(✓) Kunchit Promprat

Issue Date : 17 July 2025

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written Approval of the head of Corporate Services 3: Equipment Calibration and Testing Services.

เอกสารไม่ควบคุม



Equipment : BOD Incubator
Condition As-Received : Used Item
Reference : 2507-01460C-4

Cert. No.: 25TM1003
Page : 2 of 3

Procedure Used :-

Calibration were conducted using calibration procedure CP-OT02 based on TLAS G-20 according to direct measurement method with Data Acquisition which connected with Resistance Temperature Detector (RTD).
The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

Instrument	Serial No.	Cert. No.	Traceable	Due Date
1) Data Acquisition	MY59003411	24LM192	TPA	24 Dec 2025

2. This certificate is valid only to the item calibrated on date and place of calibration.


3. This measurement result is traceable to the International System of Unit maintained through :

Remark : TPA : Technology Promotion Association (Thailand - Japan)

Result of Calibration :- (*) Without Adjustment

Function of UUC* : Temperature Source

Fresh air setting : Not Available



Probe Installation Details :

Dimension of Chamber :	
a = 10 cm	D = 0.62 m
b = 10 cm	W = 1.2 m
c = 10 cm	H = 1.2 m
	Capacity = 0.89 m³

Environment during calibration		
	Beginning	Finished
Temp. (°C)	26	26
REL.Humid. (%)	55	57
AC Supply (Volt)	223	226

Position :	Ref. Std. ID No.:
1	25-20RTD-2/1
2	25-20RTD-2/2
3	25-20RTD-2/3
4	20RTD-2/4
5	20RTD-2/5
6	20RTD-2/6
7	20RTD-2/7
8	20RTD-2/8
9 (ref.)	20RTD-2/9



Equipment : BOD Incubator
Condition As-Received : Used Item
Reference : 2507-01460C-4
Result of Calibration :- (*) Without Adjustment
Function of UUC* : Temperature Source
Fresh air setting : Not Available

Cert. No.: 25TM1003
Page : 3 of 3

Calibration Point (°C)	UUC* Setting (°C)	UUC* Reading (°C)	Temperature stability (± °C)	Temperature uniformity (°C)	Overall Variation (°C)	Coverage Factor k
20.0	20.0	19.8	0.51	0.31	1.2	2

Calibration Point (°C)	Measured Temperature (°C)									Uncertainty (± °C)
	1	2	3	4	5	6	7	8	9 (ref.)	
20.0	19.958	19.896	20.016	20.116	19.830	19.771	19.871	19.880	19.909	0.75

Average* : The average of 30 values in each position.

Temperature stability : One-half of the greatest maximum difference of measured temperature at any one sensor.

Temperature uniformity : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.

Overall Variation : The Difference of the maximum and minimum measured temperatures throughout observation.

UUC* : Unit Under Calibration

Note : The reported uncertainty of measurement was included stability and excluded uniformity .

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k , providing a level of confidence of approximately 95 %.

-00o-

เอกสารไม่ควบคุม

เอกสารไม่ควบคุม

Verification Certificate

Certificate No.: 2501440-001-01
Client name: UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.
Address: 3 Soi Udumsuk 41, Sukhumvit Road,
Bangchack, Prakhonong, Bangkok 10260

Page 1 of 4

Equipment: Digestion Unit (Heating Block)
Manufacturer: FOSS
Model: Tecator Digester 2520
Serial No.: 91905060
ID No.: UAE.WAS.030/2566
Order No.: 2501440
Operation No.: 2501440-001
Date of Receipt: 27 January 2025
Date of Calibration: 27 January 2025

Calibrated by **Approved by**
Scientist Manager, Division of Calibration Laboratory
Responsible for the Technical Management Team
Date of Issue: 29 January 2025

The uncertainties are for a confidence probability of approximately 95 %.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the National Food Institute.

F-CS-012 Revision: 01 Date: 20-04-65

2501440-001-001-01 ฐานอาหารและพัฒนาอุตสาหกรรม ศูนย์บริการห้องปฏิบัติการอุตสาหกรรมอาหาร
2501440-001-001-01 ฐานอาหารและพัฒนาอุตสาหกรรม ศูนย์บริการห้องปฏิบัติการอุตสาหกรรมอาหาร
2501440-001-001-01 ฐานอาหารและพัฒนาอุตสาหกรรม ศูนย์บริการห้องปฏิบัติการอุตสาหกรรมอาหาร
Tel: +66(0) 2422 65689 Fax: +66(0) 2422 65645

Verification Report

Certificate No.: 2501440-001-01
Equipment: Digestion Unit (Heating Block)
Model: Tecator Digester 2520 Serial No.: 91905060
Resolution: 1 °C ID No : UAE.WAS.030/2566
Manufacturer: FOSS
27 January 2025

Page 2 of 4

Location: Dry Laboratory (312), UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.
Environment Condition: Ambient Temperature (29 ± 1) °C
Relative Humidity (58 ± 2) %
Line Voltage (224 ± 1) Volt

Condition of this results of Calibration:

- This instrument was calibrated by insert standard thermocouples type R into its Digestion blocks and Calibration according to NFI Method W-TE-026 based on BS 4309 : 1968
- The temperature scale used was based on ITS - 90 .
- All data show below were final values and the initial data may be obtained upon request.

2. Reference Standard Instrument :

Instrument	Model	Serial No.	Certificate No.	Due Date	Through
Digital Thermometer with Thermocouple	34970A Type R	MY44045576/MY41194453	TC24/0063	5-Jun-2025	N.M. Technical Center Laboratory

- This certificate is traceable to International System of Units (SI Units).
- This certificate was certified only for the instrument we calibrated.
- This result of calibration was found accurate as shown on date and place of calibration only.
- Condition of Calibrated item : Good

UUC* Description
Time of Record 1 Hour 6 Minute At 380 °C
7. Result of Calibration : ☒ Without adjustment ☐ After adjustment

F-CS-012 Revision: 01 Date: 20-04-65

2501440-001-001-01 ฐานอาหารและพัฒนาอุตสาหกรรม ศูนย์บริการห้องปฏิบัติการอุตสาหกรรมอาหาร
2501440-001-001-01 ฐานอาหารและพัฒนาอุตสาหกรรม ศูนย์บริการห้องปฏิบัติการอุตสาหกรรมอาหาร
2501440-001-001-01 ฐานอาหารและพัฒนาอุตสาหกรรม ศูนย์บริการห้องปฏิบัติการอุตสาหกรรมอาหาร
Tel: +66(0) 2422 65689 Fax: +66(0) 2422 65645

Verification Report

Certificate No.: 2501440-001-01
Equipment: Digestion Unit (Heating Block)
Model: Tecator Digester 2520 Serial No.: 91905060
Resolution: 1 °C ID No : UAE.WAS.030/2566
Manufacturer: FOSS

Date of Calibration: 27 January 2025 Page 3 of 4

Calibration point: 380 °C

Calibration result:

Table1 : Reporting of Temperature

Block No.	UUC* Setting (°C)	UUC* Reading (°C)	Stability (±°C)	Standard Thermometer (°C)	Uncertainty (±°C)
1	380	380	0.22	377.84	2.0
2	380	380	0.19	378.68	2.0
3	380	380	0.13	378.70	2.0
4	380	380	0.12	379.82	2.0
5	380	380	0.20	381.01	2.0
6	380	380	0.16	380.48	2.0
7	380	380	0.16	378.22	2.0
8	380	380	0.19	377.99	2.0
9	380	380	0.09	378.48	2.0
10	380	380	0.15	378.17	2.0
11	380	380	0.18	377.64	2.0
12	380	380	0.11	379.27	2.0
13	380	380	0.13	378.14	2.0
14	380	380	0.25	379.11	2.0
15	380	380	0.15	379.83	2.0
16	380	380	0.18	378.05	2.0
17	380	380	0.31	378.44	2.0
18	380	380	0.18	378.29	2.0
19	380	380	0.17	378.41	2.0
20	380	380	0.13	379.24	2.0

Note:

- UUC* = Unit Under Calibration
- Immersion depth of standard thermometer in tube level high of sand is equal heater plate of UUC.
- Stability = One-half of the greatest maximum difference of measured temperatures at one sensors, for at least half an hour after reaching steady state.

The report uncertainty of measurement was based on standard uncertainty multiplied by coverage factor $k = 2$, providing a level of confidence of approximately 95 %.

F-CS-012 Revision: 01 Date: 20-04-65

2501440-001-001-01 ฐานอาหารและพัฒนาอุตสาหกรรม ศูนย์บริการห้องปฏิบัติการอุตสาหกรรมอาหาร
2501440-001-001-01 ฐานอาหารและพัฒนาอุตสาหกรรม ศูนย์บริการห้องปฏิบัติการอุตสาหกรรมอาหาร
2501440-001-001-01 ฐานอาหารและพัฒนาอุตสาหกรรม ศูนย์บริการห้องปฏิบัติการอุตสาหกรรมอาหาร
Tel: +66(0) 2422 65689 Fax: +66(0) 2422 65645

Verification Report


Certificate No.: 2501440-001-01
Equipment: Digestion Unit (Heating Block)
Model: Tecator Digester ; Serial No.: 91905060
Resolution: 1 °C ID No : UAE.WAS.030/2566
Manufacturer: FOSS

Date of Calibration: 27 January 2025 Page 4 of 4

Calibration point: 380 °C

Calibration result: Continued

Figure 1. Location of Reference Standard and Block Diagram of Digestion Unit

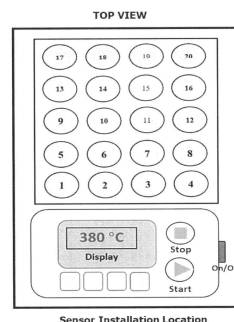

----- End -----

F-CS-012 Revision: 01 Date: 20-04-65

2501440-001-001-01 ฐานอาหารและพัฒนาอุตสาหกรรม ศูนย์บริการห้องปฏิบัติการอุตสาหกรรมอาหาร
2501440-001-001-01 ฐานอาหารและพัฒนาอุตสาหกรรม ศูนย์บริการห้องปฏิบัติการอุตสาหกรรมอาหาร
2501440-001-001-01 ฐานอาหารและพัฒนาอุตสาหกรรม ศูนย์บริการห้องปฏิบัติการอุตสาหกรรมอาหาร
Tel: +66(0) 2422 65689 Fax: +66(0) 2422 65645

DQE Services Co.,Ltd.

DQE Services

32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Bangkok 10230

Phone : +66 (0)2 538 2054, Email : dqeservicesinfo@gmail.com

ISO 17025

19252

CALIBRATION 0404

CERTIFICATE OF CALIBRATION

Certificate No. : SP25-001

Page 1 of 5

Customer : United Analyst and Engineering Consultant Co.,Ltd. (Head Office)

Address : 3 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260

Location of calibration : Laboratory 213

Equipment : UV-Vis Spectrophotometer

Manufacturer : Hitachi

Model : U-2900

Serial No. : 21E22-009

ID No. : UAE.WAT.051/2564

Received Date : 3 January 2025

Calibration Date : 3 January 2025

Issue Date : 8 January 2025

Condition Instrument : Good

Calibrated by :

Approved by :

Technical Manager

Quality Manager

The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only.

The measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of DQE Services Co., Ltd.

เอกสารไม่ควบคุม

FM-708-02 R01 1/11/2021

DQE Services Co.,Ltd.

DQE Services

32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Bangkok 10230

Phone : +66 (0)2 538 2054, Email : dqeservicesinfo@gmail.com

ISO 17025

19252

CALIBRATION 0404

REPORT OF CALIBRATION

Certificate No. : SP25-001

Page 2 of 5

Environment Condition : Ambient Temperature 25 ± 5 °C

Relative humidity 55 ± 20 %RH

Calibration method : In-house method CP-01 Based on ASTM E275-08

Certified Reference Materials :

Material	Serial No.	Certificate No.	Due date
Absorbance Standard set	25760	115663	25 October 2025
Absorbance Standard set	25757	115638	25 October 2025
Wavelength Standard set	25806	115657	25 October 2025
Wavelength Standard set	25758	115665	25 October 2025

Traceability : This certification is traceable to the International System of Unit maintained at National - Institute of Standards and Technology (NIST) through Starna Scientific Limited

Spectral Band Width of UUC : 1.5 nm.

Scan Speed of UUC : 200 nm/min

Scan Interval of UUC : 0.1 nm.

Resolution of UUC : Photometric 0.001 Abs.

Wavelength 0.1 nm.

DQE Services Co.,Ltd.

DQE Services

32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Bangkok 10230

Phone : +66 (0)2 538 2054, Email : dqeservicesinfo@gmail.com

ISO 17025

19252

CALIBRATION 0404

REPORT OF CALIBRATION

Certificate No. : SP25-001

Page 3 of 5

Calibration Results : Without adjustment

Photometric Accuracy :

Wavelength (nm.)	CRMs Values (Abs)	UUC Reading (Abs)	Correction (Abs)	Uncertainty (Abs)	Coverage factor k
420	0.0000	0.000	0.0000	0.0028	2.00
	0.5780	0.578	0.0000	0.0031	2.00
	1.0484	1.045	0.0034	0.0029	2.00
	2.1876	2.192	-0.0044	0.0075	2.00
440	0.0000	0.000	0.0000	0.0028	2.00
	0.5595	0.560	-0.0005	0.0034	2.00
	1.0239	1.023	0.0009	0.0035	2.00
	2.1230	2.125	-0.0020	0.0079	2.00
465	0.0000	0.000	0.0000	0.0028	2.00
	0.5230	0.521	0.0020	0.0030	2.00
	0.9633	0.961	0.0023	0.0029	2.00
	1.9753	1.977	-0.0017	0.0070	2.00
546.1	0.0000	0.000	0.0000	0.0028	2.00
	0.5181	0.518	0.0001	0.0031	2.00
	1.0002	0.998	0.0022	0.0033	2.00
	1.9973	1.993	0.0043	0.0084	2.00
590	0.0000	0.000	0.0000	0.0028	2.00
	0.5517	0.552	-0.0003	0.0030	2.00
	1.0803	1.079	0.0013	0.0030	2.00
	2.0373	2.032	0.0053	0.0079	2.00
635	0.0000	0.000	0.0000	0.0028	2.00
	0.5591	0.559	0.0001	0.0031	2.00
	1.0518	1.050	0.0018	0.0030	2.00
	1.9274	1.923	0.0044	0.0079	2.00

เอกสารไม่ควบคุม

FM-708-02 R01 1/11/2021

DQE Services Co.,Ltd.

DQE Services

32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Bangkok 10230

Phone : +66 (0)2 538 2054, Email : dqeservicesinfo@gmail.com

ISO 17025

19252

CALIBRATION 0404

REPORT OF CALIBRATION

Certificate No. : SP25-001

Page 4 of 5

Photometric Accuracy :

Wavelength (nm.)	CRMs Values (Abs)	UUC Reading (Abs)	Correction (Abs)	Uncertainty (Abs)	Coverage factor k
235	0.0000	0.000	0.0000	0.0050	2.00
	0.7469	0.744	0.0029	0.0057	2.00
257	0.0000	0.000	0.0000	0.0050	2.00
	0.8674	0.863	0.0044	0.0059	2.00
313	0.0000	0.000	0.0000	0.0050	2.00
	0.2919	0.290	0.0019	0.0051	2.00
350	0.0000	0.000	0.0000	0.0050	2.00
	0.6430	0.640	0.0030	0.0055	2.00

เอกสารไม่ควบคุม

FM-708-02 R01 1/11/2021

DQE Services Co.,Ltd.

DQE Services

32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Bangkok 10230

Phone : +66 (0)2 538 2054, Email : dqeservicesinfo@gmail.com



ISO 17025:2017

LABORATORY

REPORT OF CALIBRATION

Certificate No. : SP25-001

Page 5 of 5

Wavelength Accuracy :

CRMs Values (nm.)	UUC Reading (nm.)	Correction (nm.)	Uncertainty (nm.)	Coverage factor <i>k</i>
241.72	241.1	0.62	0.18	2.00
279.45	279.0	0.45	0.18	2.00
287.81	287.3	0.51	0.18	2.00
334.06	333.8	0.26	0.18	2.00
360.93	360.6	0.33	0.18	2.00
418.59	418.2	0.39	0.18	2.00
445.94	445.5	0.44	0.18	2.00
453.66	453.4	0.26	0.18	2.00
460.02	459.8	0.22	0.18	2.00
536.59	536.6	-0.01	0.18	2.00
637.98	637.7	0.28	0.18	2.00
431.38	431.1	0.28	0.18	2.00
472.50	472.3	0.20	0.18	2.00
513.47	513.4	0.07	0.18	2.00
528.88	528.9	-0.02	0.18	2.00
573.17	573.3	-0.13	0.18	2.00
585.35	585.1	0.25	0.20	2.00
684.40	684.5	-0.10	0.18	2.00
740.72	741.0	-0.28	0.20	2.00
748.55	748.8	-0.25	0.18	2.00
807.03	807.3	-0.27	0.18	2.00
879.28	879.6	-0.32	0.18	2.00

Remark : - UUC = Unit Under Calibration

- N/A = Not Available

- The result expanded uncertainty of measurement U is stated as the standard uncertainty of measurement multiplied by the coverage factor *k*, which for a normal distribution corresponds to a coverage probability of approximately 95%

- End of Certificate -

เอกสารไม่ควบคุม

FM-708-02 R01 1/11/2021

DQE Services Co.,Ltd.

DQE Services

32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Bangkok 10230

Phone : +66 (0)2 538 2054, Email : dqeservicesinfo@gmail.com



ISO 17025:2017

LABORATORY

CERTIFICATE OF CALIBRATION

Certificate No. : SP25-024

Page 1 of 5

Customer : United Analyst and Engineering Consultant Co.,Ltd. (Head Office)

Address : 3 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260

Location of calibration : Instrument room (207)

Equipment : UV-Vis Spectrophotometer

Manufacturer : HITACHI

Model : U-5100

Serial No. : 23A4-008


ID No. : UAE.WAS.010/2567

Received Date : 17 June 2025

Calibration Date : 17 June 2025

Issue Date : 20 June 2025

Condition Instrument : Good

Calibrated by : 

Approved by : 

Technical Manager

Quality Manager

The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only.

The measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the DQE Services Co., Ltd.

เอกสารไม่ควบคุม

FM-708-02 R01 1/11/2021

DQE Services Co.,Ltd.

DQE Services

32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Bangkok 10230

Phone : +66 (0)2 538 2054, Email : dqeservicesinfo@gmail.com



ISO 17025:2017

LABORATORY

REPORT OF CALIBRATION

Certificate No. : SP25-024

Page 2 of 5

Environment Condition : Ambient Temperature 25 ± 5 °C

Relative humidity 55 ± 20 %RH

Calibration method : In-house method CP-01 Based on ASTM E275-08

Certified Reference Materials :

Material	Serial No.	Certificate No.	Due date
Absorbance Standard set	25760	115663	25 October 2025
Absorbance Standard set	25757	115638	25 October 2025
Wavelength Standard set	25806	115657	25 October 2025
Wavelength Standard set	25758	115665	25 October 2025

Traceability : This certification is traceable to the International System of Unit maintained at National - Institute of Standards and Technology (NIST) through Starna Scientific Limited

Spectral Band Width of UUC : 5.0 nm.

Scan Speed of UUC : 40

Scan Interval of UUC : 0.1 nm.

Resolution of UUC : Photometric 0.001 Abs.

Wavelength 0.1 nm.

เอกสารไม่ควบคุม

FM-708-02 R01 1/11/2021

DQE Services Co.,Ltd.

DQE Services

32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Bangkok 10230

Phone : +66 (0)2 538 2054, Email : dqeservicesinfo@gmail.com



ISO 17025:2017

LABORATORY

REPORT OF CALIBRATION

Certificate No. : SP25-024

Page 3 of 5

Calibration Results : Without adjustment

Photometric Accuracy :

Wavelength (nm.)	CRMs Values (Abs)	UUC Reading (Abs)	Correction (Abs)	Uncertainty (Abs)	Coverage factor <i>k</i>
420	0.0000	0.000	0.0000	0.0028	2.00
	0.5780	0.574	0.0040	0.0031	2.00
	1.0484	1.044	0.0044	0.0029	2.00
	2.1876	2.185	0.0026	0.0075	2.00
440	0.0000	0.000	0.0000	0.0028	2.00
	0.5595	0.558	0.0015	0.0035	2.00
	1.0239	1.021	0.0029	0.0035	2.00
	2.1230	2.122	0.0010	0.0079	2.00
465	0.0000	0.000	0.0000	0.0028	2.00
	0.5230	0.519	0.0040	0.0030	2.00
	0.9633	0.961	0.0023	0.0029	2.00
	1.9753	1.975	0.0003	0.0071	2.00
546.1	0.0000	0.000	0.0000	0.0028	2.00
	0.5181	0.515	0.0031	0.0031	2.00
	1.0002	0.996	0.0042	0.0033	2.00
	1.9973	1.994	0.0033	0.0084	2.00
590	0.0000	0.000	0.0000	0.0028	2.00
	0.5517	0.549	0.0027	0.0030	2.00
	1.0803	1.078	0.0023	0.0030	2.00
	2.0373	2.031	0.0063	0.0082	2.00
635	0.0000	0.000	0.0000	0.0028	2.00
	0.5591	0.557	0.0021	0.0031	2.00
	1.0518	1.049	0.0028	0.0030	2.00
	1.9274	1.924	0.0034	0.0081	2.00

เอกสารไม่ควบคุม

FM-708-02 R01 1/11/2021

Calibration Report

Certificate No.: 2502229-004-01
Equipment: CHAMBER (Incubator)
Model: KB 400 **Serial No.:** 20200000015535
Resolution: 0.1 °C **ID No.:** UAE.MIC.018/2564
Manufacturer: BINDER

Date of Calibration: 19 March 2025
Calibration point: 35.0 °C

Calibration result:

Calibration Condition	Temperature (°C)	Relative Humidity (%)	Line Voltage (Volt)
MIN	17.1	45	220.0
MAX	18.1	55	225.0




Table 1 : Reporting of Temperature

Calibration point (°C)	Measured Temperature (°C) @ Sensor No. (Sensor No.13 is REF)													Uncertainty ± (°C)
	# 1	# 2	# 3	# 4	# 5	# 6	# 7	# 8	# 9	# 10	# 11	# 12	# 13	
35.0	34.98	35.17	34.99	34.92	35.18	35.01	35.00	35.13	35.00	34.96	35.02	35.17	35.04	0.27

Table 2 : Reporting of Characterization Result

UUC* Setting (°C)	UUC* Reading (°C)			Temperature Stability ± (°C)	Temperature Uniformity (°C)	Overall Variation (°C)
	MIN	MAX	Average			
35.0	35.0	35.0	35.0	0.029	0.15	0.30

Note: The quoted uncertainty include " Stability " and " Loading effect (20% of Temp Uniformity) "
UUC* = Unit Under Calibration
Stability = One-half of the greatest maximum difference of measured temperatures at any one sensors, for at least half an hour after reaching steady state.
Uniformity = The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time.
Overall Variation = The difference of the maximum and minimum measured temperatures throughout observation time.
The report uncertainty of measurement was based on standard uncertainty multiplied by coverage factor k=2, providing a level of confidence of approximately 95 %.

----- End -----

F-CS-012 Revision: 01 Date: 20-04-65

2008 ซอย 36 ถนนสุขุมวิท แขวงคลองตัน เขตคลองเตย กรุงเทพมหานคร
2008 Soi 36, Arun Amarin Road, Bang Yi Khan Subdistrict, Bang Phlat District, Bangkok 10700, Thailand
Tel: +66(0) 2422 8568 Fax: +66(0) 2422 8545



Calibration Certificate

Certificate No.: 2502229-004-01
Client name: UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.
Address: 3 Soi Udomsuk 41, Sukhumvit Road, Bangchack, Prakanong, Bangkok 10260

Equipment: CHAMBER (Incubator)

Manufacturer: MEMMERT

Model: IN75

Serial No.: D317.0305

ID No.: UAE.MIC.022/2561

Order No.: 2502229

Operation No.: 2502229-004

Date of Receipt: 19 March 2025

Date of Calibration: 20 March 2025

Calibrated by: Scientist **Approved by:** Manager, Division of Calibration Laboratory
Responsible for the Technical Management Team

The uncertainties are for a confidence probability of approximately 95 %.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the National Food Institute.

F-CS-009 Revision: 01 Date: 20-04-65

2008 ซอย 36 ถนนสุขุมวิท แขวงคลองตัน เขตคลองเตย กรุงเทพมหานคร
2008 Soi 36, Arun Amarin Road, Bang Yi Khan Subdistrict, Bang Phlat District, Bangkok 10700, Thailand
Tel: +66(0) 2422 8568 Fax: +66(0) 2422 8545



Calibration Report

Certificate No.: 2502229-004-01
Equipment: CHAMBER (Incubator)
Model: IN75 **Serial No.:** D317.0305
Resolution: 0.1 °C **ID No.:** UAE.MIC.022/2561
Manufacturer: MEMMERT

Date of Calibration: 20 March 2025

Location: 302, UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.
Environment Condition: Ambient Temperature (28.8 ± 1) °C
Relative Humidity (59 ± 1) %
Line Voltage (223 ± 3) Volt

Condition of this results of Calibration:

- This instrument was calibrated by insert 9 standard thermometer into its chamber and calibration according to W-TE-014 Based on TLAS G-20-1/02-08 (E): Guidelines for Calibration and Checks of Temperature Controlled Enclosures.
- The temperature scale used was based on ITS - 90.
- All data show below were final values and the initial data may be obtained upon request.
- Reference Standard Instrument :

Instrument	Model	Serial No./ID No.	Certificate No.	Due Date	Through
Digital Thermometer with sensor	34972A	MY57003188	TE 670486-01	8 June 2025	NATIONAL FOOD INSTITUTE
	RTD	CH#101-109/ RTD#101-109			

- This certificate is traceable to International System of Units (SI Units).
- This certificate was certified only for the instrument we calibrated.
- This result of calibration was found accurate as shown on date and place of calibration only.
- Condition of Calibrated item : Good

UUC Description :
Time of Record 1 Hour 9 Minute At 41.5 °C
Fresh air Damper - Open Position -
X Close Fan 100%
Not Available
7. Result of Calibration : X Without adjustment After adjustment

F-CS-012 Revision: 01 Date: 20-04-65

2008 ซอย 36 ถนนสุขุมวิท แขวงคลองตัน เขตคลองเตย กรุงเทพมหานคร
2008 Soi 36, Arun Amarin Road, Bang Yi Khan Subdistrict, Bang Phlat District, Bangkok 10700, Thailand
Tel: +66(0) 2422 8568 Fax: +66(0) 2422 8545



Calibration Report

Certificate No.: 2502229-004-01
Equipment: CHAMBER (Incubator)
Model: IN75 **Serial No.:** D317.0305
Resolution: 0.1 °C **ID No.:** UAE.MIC.022/2561
Manufacturer: MEMMERT

Date of Calibration: 20 March 2025

Calibration point: 41.5 °C

Calibration result:

Calibration Condition	Temperature (°C)	Relative Humidity (%)	Line Voltage (Volt)
MIN	28.6	58	220.0
MAX	28.9	60	225.0




Table1 : Reporting of Temperature

Calibration point (°C)	Measured Temperature (°C) @ Sensor No. (Sensor No.9 is REF)									Uncertainty ± (°C)
	# 1	# 2	# 3	# 4	# 5	# 6	# 7	# 8	# 9	
41.5	41.50	41.39	41.45	41.40	41.69	41.35	41.29	41.32	41.34	0.27

Table 2 : Reporting of Characterization Result

UUC* Setting (°C)	UUC* Reading (°C)			Stability ± (°C)	Uniformity (°C)	Overall Variation (°C)
	MIN	MAX	Average			
41.5	41.5	41.5	41.5	0.023	0.34	0.44

Note: The quoted uncertainty include " Stability " and " Loading effect (20% of Temp Uniformity) "
UUC* = Unit Under Calibration
Stability = One-half of the greatest maximum difference of measured temperatures at any one sensors, for at least half an hour after reaching steady state.
Uniformity = The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time.
Overall Variation = The difference of the maximum and minimum measured temperatures throughout observation time.
The report uncertainty of measurement was based on standard uncertainty multiplied by coverage factor k=2, providing a level of confidence of approximately 95 %.

----- End -----

F-CS-012 Revision: 01 Date: 20-04-65

2008 ซอย 36 ถนนสุขุมวิท แขวงคลองตัน เขตคลองเตย กรุงเทพมหานคร
2008 Soi 36, Arun Amarin Road, Bang Yi Khan Subdistrict, Bang Phlat District, Bangkok 10700, Thailand
Tel: +66(0) 2422 8568 Fax: +66(0) 2422 8545



Calibration Certificate

Certificate No.: 2502229-001-01
Client name: UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.
Address: 3 Soi Udomsuk 41, Sukhumvit Road,
Bangchack, Prakanong, Bangkok 10260

Page 1 of 3

Equipment: CHAMBER (Incubator)

Manufacturer: MEMMERT

Model: IPP 260

Serial No.: V615.0187

ID No.: UAE.MIC.003/2559

Order No.: 2502229

Operation No.: 2502229-001

Date of Receipt: 19 March 2025

Date of Calibration: 19 March 2025

Calibrated by **Approved by**

Scientist

Manager, Division of Calibration Laboratory

Date of Issue: 25 March 2025

Responsible for the Technical Management Team

The uncertainties are for a confidence probability of approximately 95 %.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the National Food Institute.

F-CS-009 Revision: 01 Date: 20-04-65

2502229-001-01 35 องศาเซลเซียส ห้องควบคุมอุณหภูมิ สถาบันวิจัยและพัฒนาอุตสาหกรรม
2502229-001-01 35 องศาเซลเซียส ห้องควบคุมอุณหภูมิ สถาบันวิจัยและพัฒนาอุตสาหกรรม
Tel: +66(0) 2422 8588 Fax: +66(0) 2422 8545



Calibration Report

Certificate No.: 2502229-001-01
Equipment: CHAMBER (Incubator)
Model: IPP 260 Serial No.: V615.0187
Resolution: 0.1 °C ID No.: UAE.MIC.003/2559
Manufacturer: MEMMERT

Date of Calibration: 19 March 2025 **Page 2 of 3**

Location: LABORATORY, UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.

Environment Condition: Ambient Temperature (16.2 ± 1) °C
Relative Humidity (32 ± 4) %
Line Voltage (223 ± 3) Volt

Condition of this results of Calibration:

- This instrument was calibrated by insert 9 standard thermometer into its chamber and calibration according to W-TE-014 Based on TLAS G-20-1/02-08 (E): Guidelines for Calibration and Checks of Temperature Controlled Enclosures.
- The temperature scale used was based on ITS - 90.
- All data show below were final values and the initial data may be obtained upon request.

2. Reference Standard Instrument :

Instrument	Model	Serial No./ID No.	Certificate No.	Due Date	Through
Digital Thermometer with sensor	34972A	MY49016851	TE 670477-01	4 May 2025	NATIONAL FOOD INSTITUTE
	RTD	CH#101-109/ RTD#101-109			

3. This certificate is traceable to International System of Units (SI Units).

4. This certificate was certified only for the instrument we calibrated.

5. This result of calibration was found accurate as shown on date and place of calibration only.

6. Condition of Calibrated item : Good

UUC Description :

Time of Record 1 Hour 9 Minute At 35.0 °C
Fresh air Damper - Open Position -
X Close Fan -
Not Available

7. Result of Calibration : X Without adjustment After adjustment

F-CS-012 Revision: 01 Date: 20-04-65

2502229-001-01 35 องศาเซลเซียส ห้องควบคุมอุณหภูมิ สถาบันวิจัยและพัฒนาอุตสาหกรรม
2502229-001-01 35 องศาเซลเซียส ห้องควบคุมอุณหภูมิ สถาบันวิจัยและพัฒนาอุตสาหกรรม
Tel: +66(0) 2422 8588 Fax: +66(0) 2422 8545



Calibration Report

Certificate No.: 2502229-001-01
Equipment: CHAMBER (Incubator)
Model: IPP 260 Serial No.: V615.0187
Resolution: 0.1 °C ID No.: UAE.MIC.003/2559
Manufacturer: MEMMERT

Date of Calibration: 19 March 2025

Calibration point: 35.0 °C

Calibration Condition	Temperature (°C)	Relative Humidity (%)	Line Voltage (Volt)
MIN	15.5	28	220.0
MAX	17.1	35	225.0

Table1 : Reporting of Temperature

Calibration point (°C)	Measured Temperature (°C) @ Sensor No. (Sensor No.9 is REF)									Uncertainty ± (°C)
	# 1	# 2	# 3	# 4	# 5	# 6	# 7	# 8	# 9	
35.0	34.94	34.95	34.91	34.93	35.15	35.01	34.98	35.05	35.12	0.29

Table 2 : Reporting of Characterization Result

UUC* Setting (°C)	UUC* Reading (°C)			Stability ± (°C)	Uniformity (°C)	Overall Variation (°C)
	MIN	MAX	Average			
35.0	35.0	35.0	35.0	0.10	0.21	0.35

Note The quoted uncertainty include " Stability " and " Loading effect (20% of Temp Uniformity) "

UUC* = Unit Under Calibration

Stability = One-half of the greatest maximum difference of measured temperatures at any one sensors, for at least half an hour after reaching steady state.

Uniformity = The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time.

Overall Variation = The difference of the maximum and minimum measured temperatures throughout observation time.

The report uncertainty of measurement was based on standard uncertainty multiplied by coverage factor k= 2, providing a level of confidence of approximately 95 %.

----- End -----

F-CS-012 Revision: 01 Date: 20-04-65

2502229-001-01 35 องศาเซลเซียส ห้องควบคุมอุณหภูมิ สถาบันวิจัยและพัฒนาอุตสาหกรรม
2502229-001-01 35 องศาเซลเซียส ห้องควบคุมอุณหภูมิ สถาบันวิจัยและพัฒนาอุตสาหกรรม
Tel: +66(0) 2422 8588 Fax: +66(0) 2422 8545



Hanna Instruments (Thailand) Ltd.

410/67-68 Soi Ratchadapisek 24, Ratchadapisek Rd., Samsen-nok,

Huaykwang, Bangkok 10310 Tel: 0-2541-4199 Fax: 0-2541-4198

Certificate No. : HIT-2513-0437

Page : 1 of 2

CERTIFICATE OF ANALYSIS

Equipment : Cyanuric Acid Portable Photometer
Meter Model : HI97722C **Serial No. :** 905060058111
Manufacturer : Hanna Instruments
Made in : Romania
Condition As-Received : Used Product
Reference : RE250509
Customer name : United Analyst and Engineering Consultant Co., Ltd.
3 Soi Udomsuk 41, Sukhumvit Rd., Bangchak,
Phrakhanong, Bangkok 10260
Received date : 20 March 2025
Calibrate date : 24 March 2025
Issue date : 24 March 2025
Ambient Temperature : (25 ± 2) °C
Relative Humidity : (50 ± 15) % RH
Calibrated Location : Hanna Instruments (Thailand) Ltd.

Calibrated by : ☒

Approved by :

Authorized Signatory



This certificate was certified only for the instrument we calibrated.

This result of calibration was found accurate on date and place of calibration only.

** This certificate may not be reproduced other than in full, except with the prior written **

approval of the head of Hanna Instrument (Thailand) Ltd.

เชกสารไม่ควบคุม

Condition of this result of analysis

Cal Check Standard Cuvettes Specifications :

Product code: HI97722-11 Lot number: SC0391/24

Standard cuvette	Standard Value (mg/L)	Lot Standard Deviation (mg/L)	Lot number	Best used before
A, ZERO	0	0.001	8366	April 2026
B, HI97722	20	0.207	7872	April 2026

Specifications for validation procedure:

Standard cuvette	Standard Value (mg/L)	Lot Standard Deviation (mg/L)	Lot number	Best used before
B, HI97722	20 ± 1	19 to 21	7872	April 2026

Method of Standardization

This quality is standardized using which is calibrated by adaptation of Turbidimetric Method as the following details below :

Result of analysis :

Cyanuric Acid Standard (mg/L)	Reading (mg/L)	Error (mg/L)
0	0	0
20 ± 1	20	0

** End of certificate **

เอกสารไม่ควบคุม