

ภาคผนวกที่ 5
เอกสารสอบเทียบเครื่องมือตรวจวัด

ภาคผนวกที่ 5-1
เอกสารสอบเทียบเครื่องมือตรวจวัดคุณภาพอากาศ

CERTIFICATE OF CALIBRATION

Certificate No. : COF-016-68

Page 1 of 2 Pages

MEASUREMENT ITEM : Top Load Orifice
MANUFACTURER : TISCH
MODEL/TYPE : TE-5025A
SERIAL NUMBER : 710725
ID NUMBER : -
CONDITION AS-RECEIVED : Used item
CUSTOMER : Pacific Laboratory Co., Ltd.
14/5358 Moo14, T.Bang Bua Thong, A.Bang Bua Thong,
Nonthaburi 11110, Thailand.

RECEIVED DATE : 02 May 2025
MEASUREMENT DATE : 13 May 2025
ISSUE DATE : 13 May 2025

ENVIRONMENTAL CONDITIONS:

Ambient condition in the laboratory are as follow:

Temperature	: 23.0 ± 3.0	°C
Relative Humidity	: 55.0 ± 15.0	%RH
Atmospheric Pressure	: 1010 ± 10	hPa

CALIBRATION CONDITION:

Preconditioning : 24 hours at ambient conditions.
Measurement Condition : The average values during measurement are 23.3 °C and 53.1 %RH.

NOTED: The certificate is valid only to the item calibrated on date and place of calibration.

TABULATION OF RESULTS:

The table on next page give the measured values.

Calibration procedure:

The Orifice gas flow device was calibrated against Standard Rotary Displacement Meter (Roots Meter) Model G65/IMC/W2-dp. The WI-CL-004 was used as a calibration guideline.

Traceability:

This certificate provides a traceability of the measurement to recognized the national standards, and to realization of the international system of units (SI) through the NIMT (National Metrology Institute of Thailand) via Certificate number: MW-0016-25.

Uncertainty of Measurement:

The reported uncertainty of measurement is based on the standard uncertainty multiplied by a coverage factor $k=2$, Which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty has been determined in accordance with the GUM 'Evaluation of measurement data - Guide to the expression of uncertainty in measurement'

Calibrated by:

- ☐ Mr. Sorawit Thachalad
☒ Miss Jittraporn Lertsomphol



Approved signatory:

Mr. Parinya Booncharoen
Calibration Department Manager

MEASUREMENT RESULTS:

The Orifice gas flow device was calibrated by direct comparison method with the Standard Rotary Displacement Meter (Roots Meter). The Humid air was used as a medium in the system. The standard conditions are 25°C (298.15 K) and 760 mmHg for standard temperature and standard pressure respectively.

Table 1: The results of Q Standard calibration data

Plate	Flow rate m^3/min	Pressure [Pa] mmHg	Temperature [Ta] °C	Temperature [Tm] °C	Δp_{meter} mmHg	$\Delta p_{Orifice}$ inH ₂ O	γ	Standard Flow [Q_s] m^3/min
1	0.706	753.337	23.01	22.02	50.559	1.718	1.309	0.659
2	0.999	753.260	23.23	22.54	63.590	3.318	1.819	0.914
3	1.119	753.236	23.25	22.52	43.489	4.417	2.098	1.054
4	1.168	753.147	23.32	22.75	32.399	4.968	2.225	1.116
5	1.411	753.149	23.33	22.84	29.194	7.361	2.708	1.354

Slope (m): 2.01373
 Intercept (b): -0.02108
 Correlation coefficient (r): 0.99983
 Uncertainty ($k=2$): 0.015 m^3/min

Table 2: The results of Q actual calibration data

Plate	Flow rate m^3/min	Pressure [Pa] mmHg	Temperature [Ta] °C	Temperature [Tm] °C	Δp_{meter} mmHg	$\Delta p_{Orifice}$ inH ₂ O	γ	Standard Flow [Q_a] m^3/min
1	0.706	753.337	23.01	22.02	50.559	1.718	0.822	0.661
2	0.999	753.260	23.23	22.54	63.590	3.318	1.143	0.917
3	1.119	753.236	23.25	22.52	43.489	4.417	1.318	1.057
4	1.168	753.147	23.32	22.75	32.399	4.968	1.398	1.120
5	1.411	753.149	23.33	22.84	29.194	7.361	1.702	1.358

Slope (m): 1.26127
 Intercept (b): -0.01323
 Correlation coefficient (r): 0.99983
 Uncertainty ($k = 2$): 0.015 m^3/min

End of Certificate of Calibration



CALIBRATION TEST REPORT FOR Partisol Air Sampler

Calibrated Date: 27 January 2025
Calibrated Due on: 26 January 2026

Report No: PM-202501029

Instruments Information

Description : Thermo Scientific Partisol 2025i
Sequential Air Sampler

Model : 2025i

Sample flow control and reporting : 5 - 18 LPM

Serial No. : 2025I2 0585 1402

Instrument used for calibration [STD]

Description : Flow Meter

BIOS DryCal DC-Lite

Model : DCL-M REV. 1.08


Range : 200 ml/min - 20 L/min

Serial No. : 5016

Environment : Temperature 25.5 °C Humidity: 51 %RH

Calibration Report

Filter	Set Flow Instrument (L/Min)	Current Flow Instrument reading (L/Min)	Actual Flow Reference standard (L/Min)	Error	Drift%
47 mm	15.00	15.00	14.91	-0.09	0.62
	16.67	16.67	16.58	-0.09	0.54
	18.34	18.34	18.21	-0.13	0.70

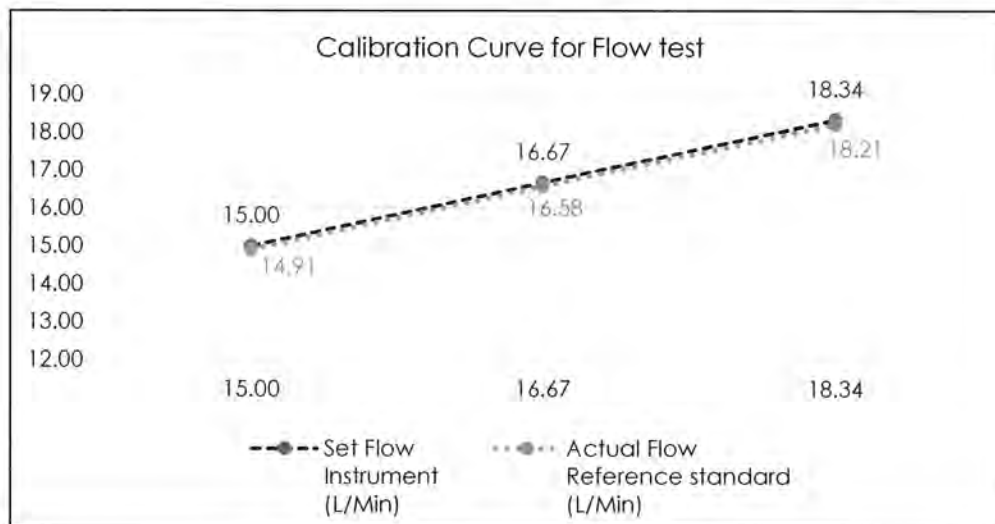

Calibrate By : 
MR. KITTISAK JANSANGWATTANA

Approve by : 
MR. PASAGORN SAMOL

ห้างหุ้นส่วนจำกัด บลู คอนซัลแตนท์ Blue Consultant Limited Partnership

32/751 ถนนประชาอุทิศ แขวงทุ่งครุ เขตทุ่งครุ กรุงเทพฯ 10140

โทร.0-2873-6045-6 โทรสาร 0-2873-6046

ห้องปฏิบัติการวิเคราะห์เอกซเรย์ใบอนุญาตลงวันที่ 22 สิงหาคม 2566

CALIBRATION REPORT

Equipment : SO₂ Analyzer

Serial No. : 1625, 2707

Brand/Model: Teledyne-API/T100

Date of Calibrate : March 12, 2025

Reference Standard

Certification Date: October 29, 2019


Component: SO₂: 55.62 ppm , NO: 57.21 ppm , CO : 4,551 ppm


Cylinder No.: EB0128767

Expiry Date: October 29, 2027

Calibration Check (Before adjust)						
Serial No.	Zero			Span		
	Reading Value (ppb)	Expected Value (ppb)	Drift (ppb)	Reading Value (ppb)	Expected Value (ppb)	Drift (ppb)
1625	0.2	0	0.2	400.9	400	0.9
2707	-0.1	0	-0.1	399.7	400	-0.3
Calibration Check (After adjust)						
Serial No.	Zero			Span		
	Reading Value (ppb)	Expected Value (ppb)	Drift (ppb)	Reading Value (ppb)	Expected Value (ppb)	Drift (ppb)
1625	0	0	0	400	400	0
2707	0	0	0	400	400	0

ในนามห้องปฏิบัติการห้างหุ้นส่วนจำกัด บลู คอนซัลแตนท์


(นางสาวนิดดา อนันต์สุวรรณชัย)
ผู้จัดการห้องปฏิบัติการ



ห้างหุ้นส่วนจำกัด บลู คอนซัลแตนท์ Blue Consultant Limited Partnership

32/751 ถนนประชาอุทิศ แขวงทุ่งครุ เขตทุ่งครุ กรุงเทพฯ 10140

โทร.0-2873-6045-6 โทรสาร 0-2873-6046

ห้องปฏิบัติการวิเคราะห์เอกซเรย์ไอออนมวลลงวันที่ 22 สิงหาคม 2566

CALIBRATION REPORT

Equipment : SO₂ Analyzer

Serial No. : 1626

Brand/Model: Teledyne-API/T100

Date of Calibrate : April 17, 2025

Reference Standard

Certification Date: October 29, 2019


Component: SO₂: 55.62 ppm , NO: 57.21 ppm , CO : 4,551 ppm

Cylinder No.: EB0128767

Expiry Date: October 29, 2027

Calibration Check (Before adjust)						
Serial No.	Zero			Span		
	Reading Value (ppb)	Expected Value (ppb)	Drift (ppb)	Reading Value (ppb)	Expected Value (ppb)	Drift (ppb)
1626	0.3	0	0.3	397.2	400	-2.8
Calibration Check (After adjust)						
Serial No.	Zero			Span		
	Reading Value (ppb)	Expected Value (ppb)	Drift (ppb)	Reading Value (ppb)	Expected Value (ppb)	Drift (ppb)
1626	0	0	0	400	400	0

ในนามห้องปฏิบัติการห้างหุ้นส่วนจำกัด บลู คอนซัลแตนท์

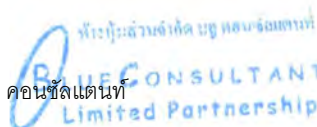

(นางสาวนิดดา อนันต์สุวรรณชัย)

ผู้จัดการห้องปฏิบัติการ

ห้างหุ้นส่วนจำกัด บลู คอนซัลแตนท์ Blue Consultant Limited Partnership

32/751 ถนนประชาอุทิศ แขวงทุ่งครุ เขตทุ่งครุ กรุงเทพฯ 10140

โทร.0-2873-6045-6 โทรสาร 0-2873-6046

ห้องปฏิบัติการวิเคราะห์เอกซเรย์อนุญาตลงวันที่ 22 สิงหาคม 2566

CALIBRATION REPORT

Equipment : NOx Analyzer

Serial No. : 99, 3205

Brand/Model: Teledyne-API/T200

Date of Calibrate : March 12, 2025

Reference Standard

Certification Date: October 29, 2019


Component: SO2: 55.62 ppm , NO: 57.21 ppm , CO : 4,551 ppm

Cylinder No.: EB0128767

Expiry Date: October 29, 2027

Calibration Check (Before adjust)						
Serial No.	Zero			Span		
	Reading Value (ppb)	Expected Value (ppb)	Drift (ppb)	Reading Value (ppb)	Expected Value (ppb)	Drift (ppb)
	NO/NO2/NOx	NO/NO2/NOx	NO/NO2/NOx	NO/NO2/NOx	NO/NO2/NOx	NO/NO2/NOx
99	-1.3/0.6/-0.7	0/0/0	-1.3/0.6/-0.7	397.7/3.4/401.1	400/0/400	-2.3/3.4/1.1
3205	3.6/1.4/5.0	0/0/0	3.6/1.4/5.0	401.2/4.1/405.3	400/0/400	1.2/4.1/5.3
Calibration Check (After adjust)						
Serial No.	Zero			Span		
	Reading Value (ppb)	Expected Value (ppb)	Drift (ppb)	Reading Value (ppb)	Expected Value (ppb)	Drift (ppb)
	NO/NO2/NOx	NO/NO2/NOx	NO/NO2/NOx	NO/NO2/NOx	NO/NO2/NOx	NO/NO2/NOx
99	0/0/0	0/0/0	0/0/0	400/0/400	400/0/400	0/0/0
3205	0/0/0	0/0/0	0/0/0	400/0/400	400/0/400	0/0/0

ในนามห้องปฏิบัติการห้างหุ้นส่วนจำกัด บลู คอนซัลแตนท์

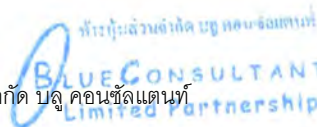

[Signature]

(นางสาวนิดดา อนันต์สุวรรณชัย)

ผู้จัดการห้องปฏิบัติการ

ห้างหุ้นส่วนจำกัด บลู คอนซัลแตนท์ Blue Consultant Limited Partnership

32/751 ถนนประชาอุทิศ แขวงทุ่งครุ เขตทุ่งครุ กรุงเทพฯ 10140

โทร.0-2873-6045-6 โทรสาร 0-2873-6046

ห้องปฏิบัติการวิเคราะห์เอกซเรย์อนุญาตลงวันที่ 22 สิงหาคม 2566

CALIBRATION REPORT

Equipment : NOx Analyzer
Serial No. : 2013

Brand/Model: Teledyne-API/T200
Date of Calibrate : April 17, 2025

Reference Standard

Certification Date: October 29, 2019


Component: SO2: 55.62 ppm , NO: 57.21 ppm , CO : 4,551 ppm

Cylinder No.: EB0128767

Expiry Date: October 29, 2027

Calibration Check (Before adjust)						
Serial No.	Zero			Span		
	Reading Value (ppb)	Expected Value (ppb)	Drift (ppb)	Reading Value (ppb)	Expected Value (ppb)	Drift (ppb)
	NO/NO2/NOx	NO/NO2/NOx	NO/NO2/NOx	NO/NO2/NOx	NO/NO2/NOx	NO/NO2/NOx
2013	4.8/1.3/6.1	0/0/0	4.8/1.3/6.1	402.2/4.6/406.8	400/0/400	2.2/4.6/6.8
Calibration Check (After adjust)						
Serial No.	Zero			Span		
	Reading Value (ppb)	Expected Value (ppb)	Drift (ppb)	Reading Value (ppb)	Expected Value (ppb)	Drift (ppb)
	NO/NO2/NOx	NO/NO2/NOx	NO/NO2/NOx	NO/NO2/NOx	NO/NO2/NOx	NO/NO2/NOx
2013	0/0/0	0/0/0	0/0/0	400/0/400	400/0/400	0/0/0

ในนามห้องปฏิบัติการห้างหุ้นส่วนจำกัด บลู คอนซัลแตนท์



.....

(นางสาวนิดดา อนันต์สุวรรณชัย)

ผู้จัดการห้องปฏิบัติการ

ห้างหุ้นส่วนจำกัด บลู คอนซัลแตนท์ Blue Consultant Limited Partnership

32/751 ถนนประชาอุทิศ แขวงทุ่งครุ เขตทุ่งครุ กรุงเทพฯ 10140

โทร.0-2873-6045-6 โทรสาร 0-2873-6046

ห้องปฏิบัติการวิเคราะห์เอกชนใบอนุญาตลงวันที่ 22 สิงหาคม 2566

CALIBRATION REPORT

Equipment : CO Analyzer
Serial No.: 48C-62630-336

Brand/Model: Thermo/48C
Date of Calibrate : April 4, 2025

Reference Standard

Cylinder No.: EB0128767

Certification Date: October 29, 2019

Expiry Date: October 29, 2027

Component: SO2: 55.62 ppm , NO: 57.21 ppm , CO : 4,551 ppm

Calibration Check (Before adjust)						
Serial No.	Zero			Span		
	Reading Value (ppm)	Expected Value (ppm)	Drift (ppm)	Reading Value (ppm)	Expected Value (ppm)	Drift (ppm)
48C-62630-336	0.2	0	0.2	40.5	40	0.5
Calibration Check (After adjust)						
Serial No.	Zero			Span		
	Reading Value (ppm)	Expected Value (ppm)	Drift (ppm)	Reading Value (ppm)	Expected Value (ppm)	Drift (ppm)
48C-62630-336	0	0	0	40	40	0

ในนามห้องปฏิบัติการห้างหุ้นส่วนจำกัด บลู คอนซัลแตนท์



(นางสาวนิดดา อนันต์สุวรรณชัย)

ผู้จัดการห้องปฏิบัติการ

ห้างหุ้นส่วนจำกัด บลู คอนซัลแตนท์ Blue Consultant Limited Partnership

32/751 ถนนประชาอุทิศ แขวงทุ่งครุ เขตทุ่งครุ กรุงเทพฯ 10140

โทร.0-2873-6045-6 โทรสาร 0-2873-6046

ห้องปฏิบัติการวิเคราะห์เอกซเรย์โพเนอูญาตลงวันที่ 22 สิงหาคม 2566

CALIBRATION REPORT

Equipment : CO Analyzer

Serial No.: 1069, 48C-62630-336

Brand/Model: API/300, Thermo/48C

Date of Calibrate : October 11, 2024

Reference Standard

Certification Date: October 29, 2019


Component: SO2: 55.62 ppm , NO: 57.21 ppm , CO : 4,551 ppm


Cylinder No.: EB0128767

Expiry Date: October 29, 2027

Calibration Check (Before adjust)						
Serial No.	Zero			Span		
	Reading Value (ppm)	Expected Value (ppm)	Drift (ppm)	Reading Value (ppm)	Expected Value (ppm)	Drift (ppm)
1069	0.2	0	0.2	39.7	40	-0.3
48C-62630-336	-0.1	0	-0.1	40.4	40	0.4
Calibration Check (After adjust)						
Serial No.	Zero			Span		
	Reading Value (ppm)	Expected Value (ppm)	Drift (ppm)	Reading Value (ppm)	Expected Value (ppm)	Drift (ppm)
1069	0	0	0	40	40	0
48C-62630-336	0	0	0	40	40	0

ในนามห้องปฏิบัติการห้างหุ้นส่วนจำกัด บลู คอนซัลแตนท์


(นางสาวนิดดา อนันต์สุวรรณชัย)
ผู้จัดการห้องปฏิบัติการ



ห้างหุ้นส่วนจำกัด บลู คอนซัลแตนท์ **Blue Consultant Limited Partnership**

32/751 ถนนประชาอุทิศ แขวงทุ่งครุ เขตทุ่งครุ กรุงเทพฯ 10140

โทร.0-2873-6045-6 โทรสาร 0-2873-6046

ห้องปฏิบัติการวิเคราะห์เอกซเรย์ไอออนธาตุลงวันที่ 22 สิงหาคม 2566

CALIBRATION REPORT

Equipment : SO₂ Analyzer

Serial No. : 2712

Brand/Model: Teledyne-API/T100

Date of Calibrate : August 14, 2025

Reference Standard

Certification Date: October 29, 2019

Component: SO₂: 55.62 ppm , NO: 57.21 ppm , CO : 4,551 ppm

Cylinder No.: EB0128767

Expiry Date: October 29, 2027

Calibration Check (Before adjust)

Serial No.	Zero			Span		
	Reading Value (ppb)	Expected Value (ppb)	Drift (ppb)	Reading Value (ppb)	Expected Value (ppb)	Drift (ppb)
2712	0.2	0	0.2	395.3	400	-4.7

Calibration Check (After adjust)

Serial No.	Zero			Span		
	Reading Value (ppb)	Expected Value (ppb)	Drift (ppb)	Reading Value (ppb)	Expected Value (ppb)	Drift (ppb)
2712	0	0	0	400	400	0

ในนามห้องปฏิบัติการห้างหุ้นส่วนจำกัด บลู คอนซัลแตนท์

(นางสาวนิดา อนันต์สุวรรณชัย)

ผู้จัดการห้องปฏิบัติการ

ห้างหุ้นส่วนจำกัด บลู คอนซัลแตนท์ Blue Consultant Limited Partnership

32/751 ถนนประชาอุทิศ แขวงทุ่งครุ เขตทุ่งครุ กรุงเทพฯ 10140

โทร.0-2873-6045-6 โทรสาร 0-2873-6046

ห้องปฏิบัติการวิเคราะห์เอกชนใบอนุญาตลงวันที่ 22 สิงหาคม 2566

CALIBRATION REPORT

Equipment : NOx Analyzer

Serial No. : 4088

Brand/Model: Teledyne-API/T200

Date of Calibrate : August 14, 2025

Reference Standard

Certification Date: October 29, 2019

Component: SO2: 55.62 ppm , NO: 57.21 ppm , CO : 4,551 ppm

Cylinder No.: EB0128767

Expiry Date: October 29, 2027

Calibration Check (Before adjust)						
Serial No.	Zero			Span		
	Reading Value (ppb)	Expected Value (ppb)	Drift (ppb)	Reading Value (ppb)	Expected Value (ppb)	Drift (ppb)
	NO/NO2/NOx	NO/NO2/NOx	NO/NO2/NOx	NO/NO2/NOx	NO/NO2/NOx	NO/NO2/NOx
4088	4.5/1.7/6.2	0/0/0	4.5/1.7/6.2	401.6/4.0/405.6	400/0/400	1.6/4.0/5.6
Calibration Check (After adjust)						
Serial No.	Zero			Span		
	Reading Value (ppb)	Expected Value (ppb)	Drift (ppb)	Reading Value (ppb)	Expected Value (ppb)	Drift (ppb)
	NO/NO2/NOx	NO/NO2/NOx	NO/NO2/NOx	NO/NO2/NOx	NO/NO2/NOx	NO/NO2/NOx
4088	0/0/0	0/0/0	0/0/0	400/0/400	400/0/400	0/0/0

ในนามห้องปฏิบัติการห้างหุ้นส่วนจำกัด บลู คอนซัลแตนท์

ห้างหุ้นส่วนจำกัด บลู คอนซัลแตนท์
BLUECONSULTANT
Limited Partnership



(นางสาวนิดดา อนันต์สุวรรณชัย)

ผู้จัดการห้องปฏิบัติการ

PERFORMANCE TEST REPORT

General Information

Instrument:	SO2 Analyzer	Report No.:	AQMCAL-008/2025
Brand / Model:	Thermo Environmental / 43C	Calibration Date:	August 3, 2025
Serial No.:	43C-65967-3510	Calibration By:	Prasert K.
Principle:	UV Fluorescence		
Measurement Range:	0 - 500 ppb		

Calibration System

Calibration Unit	Certified Gas Cylinder	Gases Concentration
Gas Dilutor: Thermo Environmental / 146C	Gas Grade: EPA Protocol	SO2 45.11 ppm
Serial No.: 00400P	Cylinder No.: LL164665	NO 45.01 ppm
Zero Air Generator: API / 701	Expired Date: 21/10/2025	CO 4511 ppm
Serial No.: 148		


Environmental Condition

Temperature (°C): 32 Relative Humidity (%): 54 Pressure (mmHg): 754

Calibration Result

Task	Gas	Unit	Zero			Span		
			SRM	Reading	Drif	SRM	Reading	Drif
Pre-cal	SO ₂	ppb	0.0	21	21	400	290	-110
Post-cal	SO ₂	ppb	0.0	0.1	0.1	400	399	-1

The calibration of the ambient air analyzer is based on the calibration procedure of US EPA published in 40 CFR Parts 50, 53 and 58.

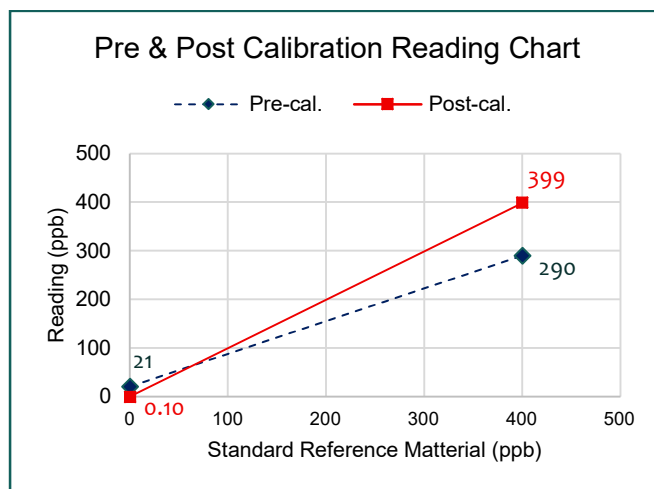

Authority Signature

(Sompong Kiatiporn)

บริษัท เอ็นควิปส์ จำกัด

หมู่บ้านกฤติกา เลขที่ 79/130 ซ.ประชาอุทิศ 4 แขวงดอนเมือง เขตดอนเมือง กรุงเทพฯ 10210

โทรศัพท์: 02 9281288 โทรสาร: 02 9281289 อีเมล: sales@enquips.com

PERFORMANCE TEST REPORT

Issued for: Pacific Laboratory Co., Ltd.

14/5358 Moo 14, Bang Bua Thong Sub-district, Bang Bua Thong District,
Nonthaburi 11110.

Calibration Instrument

Destination: Ambient Air Analyzer

Manufacture: 1) Thermo Electron Corporation, USA.

Model 43C SO₂ Analyzer

2) Thermo Electron Corporation, USA.

Model 48C CO Analyzer

This report includes: 3 pages

Date: August 3, 2025

This certificate may not be reproduced other than in full by photographic process.

ห้างหุ้นส่วนจำกัด บลู คอนซัลแตนท์ Blue Consultant Limited Partnership

32/751 ถนนประชาอุทิศ แขวงทุ่งครุ เขตทุ่งครุ กรุงเทพฯ 10140

โทร.0-2873-6045-6 โทรสาร 0-2873-6046

ห้องปฏิบัติการวิเคราะห์เอกซเรย์อนุญาตลงวันที่ 22 สิงหาคม 2566

CALIBRATION REPORT

Equipment : NOx Analyzer

Serial No. : 99, 2013

Brand/Model: Teledyne-API/T200

Date of Calibrate : March 4, 2025

Reference Standard

Certification Date: October 29, 2019

Component: SO2: 55.62 ppm , NO: 57.21 ppm , CO : 4,551 ppm

Cylinder No.: EB0128767

Expiry Date: October 29, 2027

Calibration Check (Before adjust)						
Serial No.	Zero			Span		
	Reading Value (ppb)	Expected Value (ppb)	Drift (ppb)	Reading Value (ppb)	Expected Value (ppb)	Drift (ppb)
	NO/NO2/NOx	NO/NO2/NOx	NO/NO2/NOx	NO/NO2/NOx	NO/NO2/NOx	NO/NO2/NOx
99	-1.3/0.6/-0.7	0/0/0	-1.3/0.6/-0.7	397.7/3.4/401.1	400/0/400	-2.3/3.4/1.1
2013	5.4/2.1/7.5	0/0/0	5.4/2.1/7.5	402.5/2.6/405.1	400/0/400	2.5/2.6/5.1
Calibration Check (After adjust)						
Serial No.	Zero			Span		
	Reading Value (ppb)	Expected Value (ppb)	Drift (ppb)	Reading Value (ppb)	Expected Value (ppb)	Drift (ppb)
	NO/NO2/NOx	NO/NO2/NOx	NO/NO2/NOx	NO/NO2/NOx	NO/NO2/NOx	NO/NO2/NOx
99	0/0/0	0/0/0	0/0/0	400/0/400	400/0/400	0/0/0
2013	0/0/0	0/0/0	0/0/0	400/0/400	400/0/400	0/0/0

ในนามห้องปฏิบัติการห้างหุ้นส่วนจำกัด บลู คอนซัลแตนท์



(นางสาวนิดดา อนันต์สุวรรณชัย)

ผู้จัดการห้องปฏิบัติการ

PERFORMANCE TEST REPORT

Issued for: Pacific Laboratory Co., Ltd.

14/5358 Moo 14, Bang Bua Thong Sub-district, Bang Bua Thong District,
Nonthaburi 11110.

Calibration Instrument

Destination: Ambient Air Analyzer

Manufacture: 1) Thermo Environmental Instruments, USA.
Model 48C CO Analyzer
Serial No. 48C-74291-376



This report includes: 2 pages

Date: September 7, 2025

PERFORMANCE TEST REPORT

General Information

Instrument: CO Analyzer
Brand / Model: Thermo Environmental / 48C
Serial No.: 48C-74291-376
Principle: Non-dispersive Infrared (NDIR)
Measurement Range: 0 - 50 ppm

Report No.: AQMCAL-010/2025
Calibration Date: September 7, 2025
Calibration By: Prasert K.

Calibration System

Calibration Unit

Gas Dilutor: Thermo Environmental / 146C
Serial No.: 00400P
Zero Air Generator: API / 701
Serial No.: 148

Certified Gas Cylinder

Gas Grade: EPA Protocol
Cylinder No.: LL164665
Expired Date: 21/10/2025

Gases Concentration

SO₂ 45.11 ppm
NO 45.01 ppm
CO 4511 ppm


Environmental Condition

Temperature (°C): 32 Relative Humidity (%): 55 Pressure (mmHg): 756

Calibration Result

Task	Gas	Unit	Zero			Span		
			SRM	Reading	Drift	SRM	Reading	Drift
Pre-cal.	CO	ppm	0.00	7.24	7.24	40	37.0	-3.0
Post-cal.	CO	ppm	0.00	0.00	0.0	40	40.2	0.2

The calibration of the ambient air analyzer is based on the calibration procedure of US EPA published in 40 CFR Parts 50, 53 and 58.

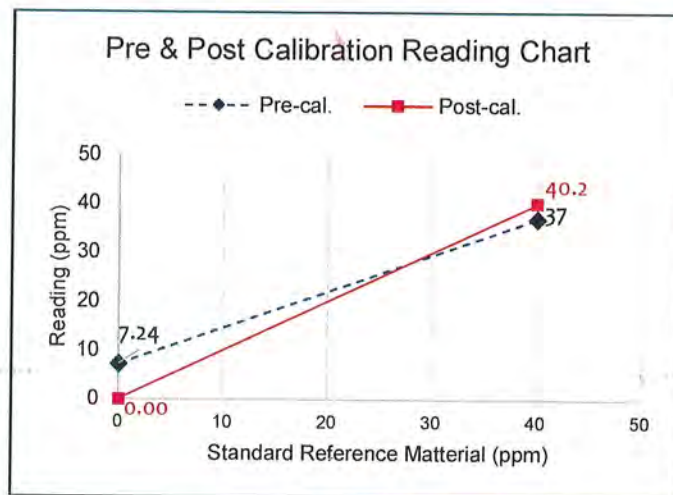

Authority Signature

(Sompong Kiatiporn)

PERFORMANCE TEST REPORT

General Information

Instrument: CO Analyzer
Brand / Model: Thermo Environment / 48C
Serial No.: 0604815184
Principle: Non-dispersive Infrared (NDIR)
Measurement Range: 0 - 50 ppm

Report No.: AQMCAL-009/2025
Calibration Date: August 12, 2025
Calibration By: Prasert K.

Calibration System

Calibration Unit

Gas Dilutor: Thermo Environmental / 146C
Serial No.: 00400P
Zero Air Generator: API / 701
Serial No.: 148

Certified Gas Cylinder

Gas Grade: EPA Protocol
Cylinder No.: LL164665
Expired Date: 21/10/2025

Gases Concentration

SO₂ 45.11 ppm
NO 45.01 ppm
CO 4511 ppm

Environmental Condition

Temperature (°C): 25.3


Relative Humidity (%): 56

Pressure (mmHg): 754

Calibration Result

Task	Gas	Unit	Zero			Span		
			SRM	Reading	Drif	SRM	Reading	Drif
Pre-cal.	CO	ppm	0.00	1.130	1.130	40	44.4	4.4
Post-cal.	CO	ppm	0.00	0.021	0.021	40	40.4	0.4

The calibration of the ambient air analyzer is based on the calibration procedure of US.EPA published in 40 CFR Parts 50, 53 and 58.

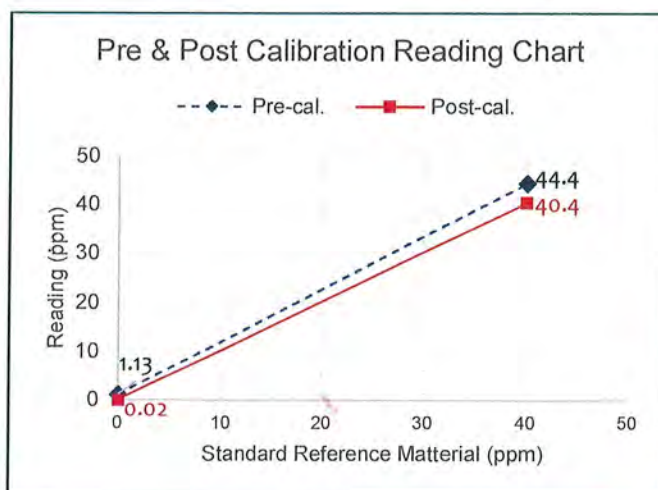

Authority Signature

(Sompong Kiatiporn)



PERFORMANCE TEST REPORT

Issued for: Pacific Laboratory Co., Ltd.

14/5358 Moo 14, Bang Bua Thong Sub-district, Bang Bua Thong District,
Nonthaburi 11110.

Calibration Instrument

Destination: Ambient Air Analyzer

Manufacture: 1) Thermo Electron Corporation, USA.

Model 48C CO Analyzer

s/n: 0604815184



This report includes: 2 pages

Date: August 12, 2025

This certificate may be reproduced other than in full by photographic process.

CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhprachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech.cal@yahoo.com, calibratech.cal@hotmail.com



NSC-TISI-TIS 17025
CALIBRATION 0030

Certificate of Calibration

Certificate No. : 67-200273-1

Page : 1 of 2

Submitted by : Pacific Laboratory Co., Ltd.

14/5358 Moo 14, T.Bang Bua Thong, A.Bang Bua Thong, Nonthaburi 11110 Thailand

Equipment : Electronic Balance

Manufacturer : SHIMADZU

Model : AP225WD

Serial No. : D316301828

ID No. : LAB-BL-003

Capacity : 220000 mg

Resolution : 0.01mg/102000mg, 0.1mg/220000mg

Environment : On site calibration was carried out at the Laboratory, Pacific Laboratory Co., Ltd.

Ambient Temperature : (26.2 to 26.4) °C

Relative Humidity : (34.0 to 35.4) %

Air Pressure : 1007.0 mbar

Date of Received : 30 July 2024

Date of Calibration : 30 July 2024

Date of Issue : 31 July 2024

Calibrated by : Akaradath Thippichai

Calibration Method : In-house method CAL-M2001 based on UKAS Publication ref : LAB 14

Edition 7 - November 2022

Reference Standard Instruments : This certification is traceable to the International System of Units

Standard Weights

ID No.	Cert. No.	Due Date	Traceability
E261-E2624	C02232088	08 Nov 2024	National Institute of Metrology (Thailand), (NIMT)

Approved by :

(Surachai Promthong)

Laboratory Manager

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhaprachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech.cal@yahoo.com, calibratech.cal@hotmail.com

Certificate of Calibration

Certificate No. : 67-200273-1

Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Departure of indication from nominal value

Nominal Value (mg)	Correction (mg)	Uncertainty \pm (mg)
1	0.01	0.012
10	0.01	0.012
50	0.01	0.012
100	0.01	0.014
1000	0.00	0.026
2000	0.01	0.034
5000	0.00	0.043
20000	0.00	0.071
50000	0.01	0.11
100000	0.00	0.20
150000	0.0	0.38
200000	0.0	0.38


This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2.06$, providing a level of confidence of approximately 95%

Eccentric error

Load test : 50000 mg

A	B	C	D	E	
0.00	0.00	0.01	0.00	0.00	mg



Repeatability

Load test : 200000 mg

Stdev. : 0.053 mg

181

- o0o -



Certificate of Calibration

Certificate No. : 68-200468-1

Page : 1 of 2

Submitted by : Pacific Laboratory Co.,Ltd.

14/5358 Moo 14, T.Bang Bua Thong, A.Bang Bua Thong, Nonthaburi 11110 Thailand

Equipment : Electronic Balance

Manufacturer : SHIMADZU

Model : AP225WD

Serial No. : D316301828

ID No. : LAB-BL-003

Capacity : 220000 mg

Resolution : 0.01mg/102000mg, 0.1mg/220000mg

Environment : On site calibration was carried out at the Laboratory, Pacific Laboratory Co.,Ltd.

Ambient Temperature : (27.3 to 27.4) °C

Relative Humidity : (53.6 to 53.7) %

Air Pressure : 1003.0 mbar

Date of Received : 21 July 2025

Date of Calibration : 21 July 2025

Date of Issue : 25 July 2025

Calibrated by : Akaradath Thippichai

Calibration Method : In-house method CAL-M2001 based on UKAS Publication ref : LAB 14

Edition 7 - November 2022

Reference Standard Instruments : This certification is traceable to the International System of Units

Standard Weights

ID No.	Cert. No.	Due Date	Traceability
E261-E2624	C02242009	07 Nov 2025	National Institute of Metrology (Thailand), (NIMT)

Approved by :

(Satja Sangkhun)

Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 68-200468-1

Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Departure of indication from nominal value


Nominal Value (mg)	Correction (mg)	Uncertainty \pm (mg)
1	0.01	0.012
10	0.00	0.012
50	0.01	0.012
100	0.01	0.014
1000	0.00	0.026
2000	0.01	0.034
5000	0.00	0.043
20000	0.00	0.071
50000	0.01	0.11
100000	0.00	0.20
150000	0.0	0.38
200000	0.0	0.38

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2.06$, providing a level of confidence of approximately 95%

Eccentric error Load test : 50000 mg

A	B	C	D	E	
0.01	0.01	0.02	0.02	0.00	mg



Repeatability Load test : 200000 mg

Stdev. : 0.053 mg

- o0o -




TEST REPORT

CUSTOMER NAME	: Pacific Laboratory Co., Ltd.						
EQUIPMENT NAME	: THC Analyzer						
MANUFACTURER	: HORIBA	MODEL	: APHA-370	SERIAL NO	: 3TEBP31U		
STANDARD GAS CONCENTRATION (PPM) (CH ₄)	: 506.1 PPM			CYLINDER NO	: CC734373		
CYLINDER PRESSURE (psig)	: 1,600 PSI			CERTIFIED DATE	: 12/05/2020		
CERTIFIED BY	: AIRGAS			EXPIRED DATE	: 12/05/2028		

TEST RESULTS

POINT NO	TEST RESULTS						
	IDEAL	ACTUAL CH ₄	ERROR CH ₄	%ERROR CH ₄	ACTUAL THC	ERROR THC	%ERROR THC
ZERO	0.00	0.00	0.00	-	0.00	0.00	-
1	10.00	10.09	0.09	0.90	10.01	0.01	0.10
2	20.00	20.04	0.04	0.20	20.09	0.09	0.45
3	30.00	30.66	0.66	2.20	30.07	0.07	0.23
4	40.00	39.99	-0.01	-0.02	40.00	0.00	0.00
AVERAGE (%)				0.82			0.20

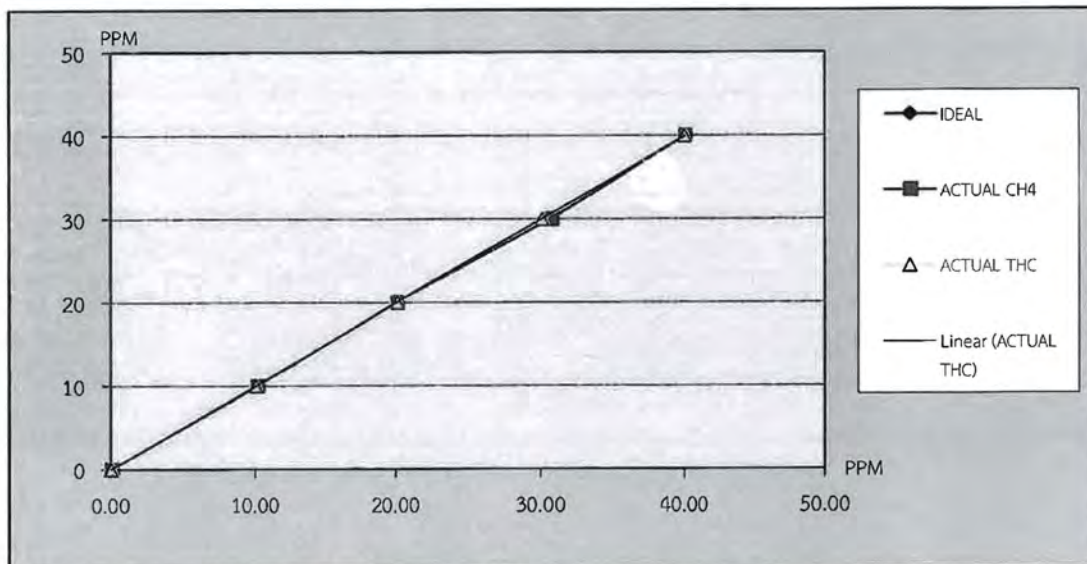

CALIBRATED BY :


อ.จ.พงศ์

DATE :

3/7/68

CHECKED BY :

ส.ร. วัฒนา



DATE :

3/7/68


ต้องการข้อมูลทางด้านเทคนิคเพิ่มเติม : เจ้าหน้าที่ฝ่ายบริการหลังการขาย , โทร 02-868-0812 # 15,16 , E-Mail : Engineer@jiranatee.com
เลขที่ 63/14-15,67/35-36 ถนนเพชรเกษม 7,7/1 แขวงวัดท่าพระ เขตบางกอกใหญ่ กรุงเทพฯ 10600 โทร 02-8680812-13 โทรสาร 02-868-1889

TEST REPORT

CUSTOMER NAME	: Pacific Laboratory Co., Ltd.						
EQUIPMENT NAME	: THC Analyzer						
MANUFACTURER	: HORIBA	MODEL	: APHA-370	SERIAL NO	: 3TEBP31U		
STANDARD GAS CONCENTRATION (PPM) (Propane)	200 PPM			CYLINDER NO	: D621701		
CYLINDER PRESSURE (psig)	: 1,900 PSI			CERTIFIED DATE	: 27/06/2018		
CERTIFIED BY	: Linde			EXPIRED DATE	: 27/06/2026		


TEST RESULTS

POINT NO	TEST RESULTS						
	IDEAL	ACTUAL NMHC	ERROR NMHC	%ERROR NMHC	ACTUAL THC	ERROR THC	%ERROR THC
ZERO	0.00	0.00	0.00	-	0.01	0.01	-
1	10.00	10.09	0.09	0.90	10.00	0.00	0.00
2	20.00	20.10	0.10	0.50	20.20	0.20	1.00
3	30.00	30.20	0.20	0.67	30.10	0.10	0.33
4	40.00	40.02	0.02	0.05	40.03	0.03	0.08
AVERAGE (%)				0.53			0.35

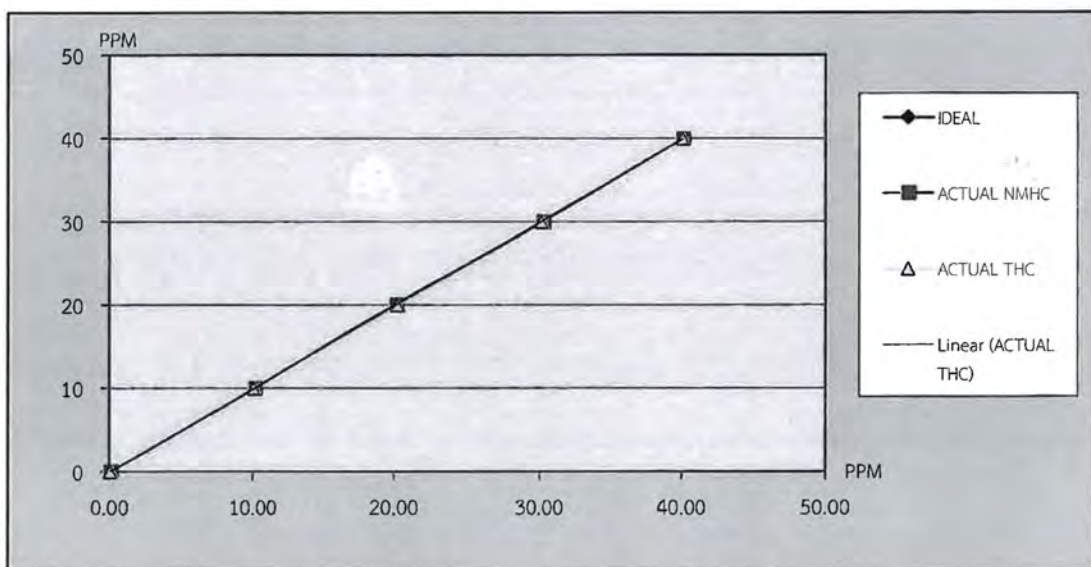

CALIBRATED BY :

ผู้พิงค์



DATE :

3/7/68

CHECKED BY :

ผู้พิงค์

DATE :

3/7/68

ต้องการข้อมูลทางด้านเทคนิคเพิ่มเติม : เจ้าหน้าที่ฝ่ายบริการหลังการขาย , โทร 02-868-0812 # 15,16 , E-Mail : Engineer@jiranatee.com
เลขที่ 63/14-15,67/35-36 ถนนเพชรเกษม 7/1 แขวงวัดท่าพระ เขตบางกอกใหญ่ กรุงเทพฯ 10600 โทร 02-8680812-13 โทรสาร 02-868-1889

CHECK LIST

CUSTOMER NAME	: Pacific Laboratory Co., Ltd.		
EQUIPMENT NAME	: THC Analyzer		
MANUFACTURER	: HORIBA	MODEL : APHA-370	SERIAL NO. : 3TEBP31U

TEST VALUES				
NO.	THC Analyzer (APHA - 370)	UNIT	BEFORE	AFTER
1	Signal (CH4)	mV	41.20	25.20
2	Signal (THC)	mV	52.80	30.70
3	Detector	Temp °C , Standard Value : Ambient temp+(5°Cto15°C)	36.70	42.90
		Pressure kPa , Standard Value : (Ambient/1013x100-20)+4kPa	81.20	80.90
4	Ambient	kPa current atmospheric pressure	101.10	100.70
5	Purifire	°C , Standard Value : 390 °C to 430 °C	271.10	419.70
		kPa , Normal value : 8 kPa to 25 kPa	9.60	9.60
6	NMHC	°C , Standard Value : 230 °C to 260 °C	117.90	234.70
7	DC 24 V	V , Standard Value : 24 V ± 0.5 V	23.90	23.90
8	DC 5 V	V , Standard Value : 5 V ± 0.5 V	5.00	5.00
9	Bypass (Optional)	L/min, Normal value : 0.9 L/min ± 0.3 L/min	-	-
10	Over Flow (Optional)	L/min, Standard Value : 0.8 L/min or More	-	-
11	CH4 Sampling Reading	PPM	3.55	2.28
12	NMHC Sampling Reading	PPM	0.39	0.39
13	THC Sampling Reading	PPM	3.99	2.67
14	Zero Gas CH4/THC	PPM	0.01/-0.02	0.00/0.00
15	Span Gas	PPM	39.82/36.12	39.99/40.00
G	Gas H2/.....	20 PSI	20	20

Remark : Reference EX-EN-017-56 , Ambient HC Monitor APHA-370 Operation Manual Page #81

Remark : (Ambient temperature = 5°C to 40°C)

อาการที่ตรวจพบ

- Service Maintenance.

รายละเอียดการดำเนินการ

- ทำ Calibration Zero/Span , Multipoint

ผลการดำเนินการ

- เรียบร้อย เครื่องสามารถดำเนินการตรวจวัดได้ตามปกติ

CALIBRATED BY : *ณัฐพงศ์*

CHECKED BY : *ณัฐพงศ์* *อรรณพ*



DATE : *3/7/68*

DATE : *3/7/68*

ต้องการข้อมูลทางด้านเทคนิคเพิ่มเติม : เจ้าหน้าที่ฝ่ายบริการหลังการขาย , โทร 02-868-0812 # 15-16 , E-Mail : Engineer@jiranatee.com

เลขที่ 63/14-15,67/35-36 ซอยเพชรเกษม 7,7/1 ถนนเพชรเกษม แขวงวัดท่าพระ เขตบางกอกใหญ่ กรุงเทพฯ 10600 โทร 02-868-0812-13 โทรสาร 02-868-1889

ภาคผนวกที่ 5-2
เอกสารสอบเทียบเครื่องมือตรวจวัดระดับเสียง



Professional Calibration & Services Co., Ltd.

50/888, 50/889 Moo 2, Rungsit-Nakornnayok Rd., Bungyeetho, Thunyaburi,
Pathumthani 12130 Thailand
Tel : (+66)2150-6641 (Autoline), (+66)2569-5158
Email : info@p-cal.com www.p-cal.com



Certificate of Calibration

Certificate Number : EL41650/24
Control Number : PCAL153035
Customer Control : -
Description : Sound Calibrator
Manufacturer : SOUNDTEK
Model : ST-120
Serial Number : 211203764
Customer : Pacific Laboratory Co., Ltd.
14/5358 Moo 14, Tambol Bang Bua Thong, Amphoe Bang Bua Thong,
Nonthaburi 11110

Date of Receipt : 22-Aug-24
Date of Calibration : 23-Aug-24
Environment : Temperature $23^{\circ}\text{C} \pm 2^{\circ}\text{C}$
Relative Humidity $50\% \pm 20\%$
Calibration Method : Calibration Procedure Number CP-EL35
Calibration Results : See data attached

Page 1 of 3



The reported uncertainty is based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%.

This certificate is issued in accordance with ISO/IEC17025 and the conditions of accreditation granted by the Accreditation Body which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory. The results relate only to the item calibrated.

This certificate shall not be reproduced other than in full except without the prior written approval of the Head of Calibration Laboratory of Professional Calibration & Services Co., Ltd.

Calibrated By

Mr. Nonpawit Wiseshoo

Authorized Signature

(Mr. Manote Piwnimnual)

27-Aug-24

Issued Date

CALIBRATION REPORT

Professional Calibration & Services Co.,Ltd.

Certificate Number : EL41650/24

Page 2 of 3

Equipment Standards Used

Description	Serial No.	Traceability to	Certificate No.	Cal. Due Date
Sound Level Meter	030606101	ANAB : AC-2590	EL12298/24	27-Mar-25
Sound Calibrator	125626778	NSC : Calibration 0037	EEL.BP. 161/0167	04-Feb-25

Condition as received : Normal

Definitions :-

- * ANAB - The ANSI National Accreditation Board
- * NSC - National Standardization Council of Thailand

CALIBRATION REPORT

Professional Calibration & Services Co., Ltd.

Certificate No.: EL41650/24

Page : 3 of 3

Calibration Results

Sound Pressure Level Accuracy

Nominal Value	Measured Value	UUC Error	Uncertainty (±)
94 dB	93.97 dB	0.03 dB	0.17 dB
114 dB	114.30 dB	-0.30 dB	0.17 dB

...End...



Professional Calibration & Services Co., Ltd.

50/888, 50/889 Moo 2, Rungsi-Nakornnayok Rd., Bungeeetho, Thunyaburi,
Pathumthani 12130 Thailand
Tel : (+66)2150-6641 (Autoline)
Email : info@p-cal.com www.p-cal.com



Certificate of Calibration

Certificate Number : EL40431/25
Control Number : PCAL153035
Customer Control : -
Description : Sound Calibrator
Manufacturer : SOUNDTEK
Model : ST-120
Serial Number : 211203764
Customer : Pacific Laboratory Co., Ltd.

Page 1 of 3



14/5358 Moo 14, Tambol Bang Bua Thong, Amphoe Bang Bua Thong,
Nonthaburi 11110

Date of Receipt : 16-Jul-25
Date of Calibration : 16-Jul-25
Calibration Location : Electrical Laboratory
Environment : Temperature $23^{\circ}\text{C} \pm 2^{\circ}\text{C}$
: Relative Humidity $50\% \pm 20\%$
Calibration Method : Calibration Procedure Number CP-EL35
Calibration Results : See data attached

The reported uncertainty is based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%.

This certificate is issued in accordance with ISO/IEC17025 and the conditions of accreditation granted by the Accreditation Body which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory. The results relate only to the item calibrated.

This certificate shall not be reproduced other than in full except without the prior written approval of the Head of Calibration Laboratory of Professional Calibration & Services Co., Ltd.

Calibrated By

Ms. Janjira Intapat

Authorized Signature

(Mr. Jinnong Junphong)

23-Jul-25

Issued Date



Professional Calibration & Services Co., Ltd.

50/888, 50/889 Moo 2, Rungsit-Nakornnayok Rd., Bungeeetho, Thunyaburi,
Pathumthani 12130 Thailand
Tel : (+66)2150-6641 (Autoline)
Email : info@p-cal.com www.p-cal.com



Calibration Report

Certificate Number : EL40431/25

Page 2 of 3

Equipment Standards Used

Description	Serial No.	Traceability to	Certificate No.	Cal. Due Date
Sound Level Meter	030606101	ANAB : AC-2590	EL11791/25	11-Mar-26
Sound Calibrator	125626778	NSC : Calibration 0037	EEL.BP. 99/0168	23-Jan-26

Condition as received : Normal

Definitions :-

- * ANAB - The ANSI National Accreditation Board
- * NSC - National Standardization Council of Thailand



Professional Calibration & Services Co., Ltd.

50/888, 50/889 Moo 2, Rungsit-Nakornnayok Rd., Bungeetho, Thunyaburi,
Pathumthani 12130 Thailand
Tel : (+66)2150-6641 (Autoline)
Email : info@p-cal.com www.p-cal.com



Calibration Report

Certificate No.: EL40431/25

Page : 3 of 3

Calibration Results

Sound Pressure Level Accuracy

Nominal Value	Measured Value	UUC Error	Uncertainty (±)
94 dB	94.01 dB	-0.01 dB	0.18 dB
114 dB	114.08 dB	-0.08 dB	0.17 dB

...End...



APTITECH CALIBRATION CO., LTD.

50/40 Moo 5 T. Lat Sawai, A. Lam Lukka, Pathumthani 12150
Tel. +66 2103-6290 Fax. +66 2103-6291
Email. sales@aptitech-cal.com



CERTIFICATE OF CALIBRATION

Certificate Number : SC240209

Customer : Pacific Laboratory Co.,Ltd.
Address : 14/5358 Moo 14 Tambol Bang Bua Thong, Amphoe Bang Thong,
Nonthaburi 11110

Description	: Sound Level Meter	W/O Number	: SC240209
Manufacturer	: Scarlet Tech	Calibration Location	: Laboratory
Model	: ST-11D	Ambient Temperature	: 22 ± 2 °C
Serial Number	: 820968	Ambient Humidity	: 55 ± 15 %RH
ID. Number	: N/A	Received Date	: 20-Aug-2024

This certifies that the above instrument was calibrated in compliance with the Calibration Systems Requirement of ISO/IEC 17025:2017 in accordance with referenced procedures. Standards used to perform this calibration are certified by or traceable to National Institute of Metrology (Thailand) and/or other recognized national measurement institutes which realizes the units of measurement according to the International System of Units (SI Unit).

Measurement uncertainties at the time of test are given where applicable. They are calculated in accordance with the method described in The Expression of Uncertainty and Confidence in Measurement (M3003).

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by coverage factor $k=2$ such that the coverage probability corresponds to approximately 95%. This result of calibration was found accurate as shown on date and place of calibration only.

Standard Equipments

Description	Serial No.	Certificate No.	Traceability	Due Date
Sound Level Calibrator	141011576	CP20240179EA	TISI: 22-LB0119	14-May-25

Authority of Calibration

Approved Signatory

- ☒ Mr. Anuwat Simsiriwat [Laboratory Manager]
☐ Mr. Nattaphol Boonmee [Quality Manager]

Calibration Date : 21-Aug-2024

Issued Date : 24-Aug-2024

Calibrated By : Ms. Hathaichanok Kaewsrisai

Calibration certificates without signatures are not valid. This certificate applied to only the item identified and shall not be reproduced other than in full, without the specific written approval by APTITECH CALIBRATION CO., LTD.



APTITECH CALIBRATION CO., LTD.

50/40 Moo 5 T. Lat Sawai, A. Lamlukka, Pathumthani 12150
Tel. +66 2103-6290 Fax. +66 2103-6291
Email. sales@aptitech-cal.com



CALIBRATION REPORT

Certificate Number : SC240209

Calibration Method

The Unit Under Calibration (UUC) was calibrated by comparison measurement with sound level calibrator. The calibration has been accomplished in an ambient environment controlled, base on the in-house calibration procedure. The identification of the laboratory's calibration procedure employed are CP-7.2-01-107

Calibration Results

Appearance and function of use : Good
Results of Calibration : Without any adjustment
Sound Level Calibration
- Frequency Weighting : A
- Resolution : 0.1 dB

Sound Level Measurement (Slow Mode)

Parameter	UUC Range	Standard Value	UUC Reading	UUC Error	(±) Uncertainty
LFp	20-140 dB	93.86 dB	93.6 dB	-0.26 dB	0.60 dB
		113.87 dB	113.6 dB	-0.27 dB	0.60 dB
LSp	20-140 dB	93.86 dB	93.6 dB	-0.26 dB	0.60 dB
		113.87 dB	113.6 dB	-0.27 dB	0.60 dB
Llp	20-140 dB	93.86 dB	93.6 dB	-0.26 dB	0.60 dB
		113.87 dB	113.6 dB	-0.27 dB	0.60 dB

Sound Level Measurement (Fast Mode)


Parameter	UUC Range	Standard Value	UUC Reading	UUC Error	(±) Uncertainty
LFp	20-140 dB	93.86 dB	93.6 dB	-0.26 dB	0.60 dB
		113.87 dB	113.5 dB	-0.37 dB	0.60 dB
LSp	20-140 dB	93.86 dB	93.6 dB	-0.26 dB	0.60 dB
		113.87 dB	113.5 dB	-0.37 dB	0.60 dB
Llp	20-140 dB	93.86 dB	93.6 dB	-0.26 dB	0.60 dB
		113.87 dB	113.5 dB	-0.37 dB	0.60 dB

--- End of Certificate ---



APTITECH CALIBRATION CO., LTD.

50/40 Moo 5 T. Lat Sawai, A. Lamlukka, Pathumthani 12150
Tel. +66 2103-6290 Fax. +66 2103-6291
Email. sales@aptitech-cal.com



CERTIFICATE OF CALIBRATION

Certificate Number : EI250284

Customer : Pacific Laboratory Co., Ltd.
Address : 14/5358 Moo 14 Tambol Bang Bua Thong Amphoe Bang Thong, Nonthaburi 11110

Description	: Sound Level Meter	W/O Number	: EI250284
Manufacturer	: Scarlet Tech	Calibration Location	: Laboratory
Model	: ST-11D	Ambient Temperature	: 22 ± 2 °C
Serial Number	: 820967	Ambient Humidity	: 55 ± 15 %RH
ID. Number	: N/A	Received Date	: 31-Jan-2025

This certifies that the above instrument was calibrated in compliance with the Calibration Systems Requirement of ISO/IEC 17025:2017 in accordance with referenced procedures. Standards used to perform this calibration are certified by or traceable to National Institute of Metrology (Thailand) and/or other recognized national measurement institutes which realizes the units of measurement according to the International System of Units (SI Unit).

Measurement uncertainties at the time of test are given where applicable. They are calculated in accordance with the method described in The Expression of Uncertainty and Confidence in Measurement (M3003).

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by coverage factor $k=2$ such that the coverage probability corresponds to approximately 95%. This result of calibration was found accurate as shown on date and place of calibration only.

Standard Equipments

Description	Serial No.	Certificate No.	Traceability	Due Date
Sound Level Calibrator	141011576	CP20240179EA	TISI: 22-LB0119	14-May-25

APTITECH

Authority of Calibration

Approved Signatory

Calibration Date : 03-Feb-2025

Issued Date : 06-Feb-2025

Calibrated By : Ms. Hathaichanok Kaewsrissai


- ☒ Mr. Anuwat Simsiriwat [Laboratory Manager]
☐ Mr. Kornupong Suksamran [Technical Manager]

Calibration certificates without signatures are not valid. This certificate applied to only the item identified and shall not be reproduced other than in full, without the specific written approval by APTITECH CALIBRATION CO., LTD.



APTITECH CALIBRATION CO., LTD.

50/40 Moo 5 T. Lat Sawai, A. Lamlukka, Pathumthani 12150
Tel. +66 2103-6290 Fax. +66 2103-6291
Email. sales@aptitech-cal.com



CALIBRATION REPORT

Certificate Number : EI250284

Calibration Method

The Unit Under Calibration (UUC) was calibrated by comparison measurement with sound level calibrator. The calibration has been accomplished in an ambient environment controlled, base on the in-house calibration procedure. The identification of the laboratory's calibration procedure employed are CP-7.2-01-107

Calibration Results

Appearance and function of use : Good
Results of Calibration : Without any adjustment
Sound Level Calibration
- Frequency Weighting : A
- Resolution : 0.1 dB

Sound Level Measurement (Slow Mode)

Parameter	UUC Range	Standard Value	UUC Reading	UUC Error	(±) Uncertainty
LFp	20-140 dB	93.86 dB	93.8 dB	-0.06 dB	0.60 dB
		113.87 dB	113.6 dB	-0.27 dB	0.60 dB
LSp	20-140 dB	93.86 dB	93.9 dB	0.04 dB	0.60 dB
		113.87 dB	113.6 dB	-0.27 dB	0.60 dB
Llp	20-140 dB	93.86 dB	93.8 dB	-0.06 dB	0.60 dB
		113.87 dB	113.5 dB	-0.37 dB	0.60 dB

Sound Level Measurement (Fast Mode)

Parameter	UUC Range	Standard Value	UUC Reading	UUC Error	(±) Uncertainty
LFp	20-140 dB	93.86 dB	93.8 dB	-0.06 dB	0.60 dB
		113.87 dB	113.7 dB	-0.17 dB	0.60 dB
LSp	20-140 dB	93.86 dB	93.8 dB	-0.06 dB	0.60 dB
		113.87 dB	113.6 dB	-0.27 dB	0.60 dB
Llp	20-140 dB	93.86 dB	93.9 dB	0.04 dB	0.60 dB
		113.87 dB	113.6 dB	-0.27 dB	0.60 dB

--- End of Certificate ---



Professional Calibration & Services Co., Ltd.

50/888, 50/889 Moo 2, Rungsit-Nakornnayok Rd., Bungyeetho, Thunyaburi,
Pathumthani 12130 Thailand
Tel : (+66)2150-6641 (Autoline)
Email : info@p-cal.com www.p-cal.com



Certificate of Calibration

Certificate Number : EL40429/25
Control Number : PCAL193431
Customer Control : -
Description : Sound Level Meter
Manufacturer : Scarler Tech
Model : ST-11D
Serial Number : 820968
Customer : Pacific Laboratory Co., Ltd.

Page 1 of 3



14/5358 Moo 14, Tambol Bang Bua Thong, Amphoe Bang Bua Thong,
Nonthaburi 11110

Date of Receipt : 16-Jul-25
Date of Calibration : 16-Jul-25
Calibration Location : Electrical Laboratory
Environment : Temperature $23^{\circ}\text{C} \pm 2^{\circ}\text{C}$
: Relative Humidity $50\% \pm 20\%$
Calibration Method : Calibration Procedure Number CP-EL35
Calibration Results : See data attached

The reported uncertainty is based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%.

This certificate is issued in accordance with ISO/IEC17025 and the conditions of accreditation granted by the Accreditation Body which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory. The results relate only to the item calibrated.

This certificate shall not be reproduced other than in full except without the prior written approval of the Head of Calibration Laboratory of Professional Calibration & Services Co., Ltd.

Calibrated By

Ms. Janjira Intapat

Authorized Signature

(Mr. Jumnonng Junphong)

23-Jul-25

Issued Date



Professional Calibration & Services Co., Ltd.

50/888, 50/889 Moo 2, Rungsit-Nakornnayok Rd., Bungyeetho, Thunyaburi,
Pathumthani 12130 Thailand
Tel : (+66)2150-6641 (Autoline)
Email : info@p-cal.com www.p-cal.com



Calibration Report

Certificate Number : EL40429/25

Page 2 of 3

Equipment Standards Used

Description	Serial No.	Traceability to	Certificate No.	Cal. Due Date
Sound Calibrator	125626778	NSC : Calibration 0037	EEL.BP. 99/0168	23-Jan-26

Condition as received : Normal

Definitions :-

* NSC - National Standardization Council of Thailand



Professional Calibration & Services Co., Ltd.

50/888, 50/889 Moo 2, Rungsit-Nakornnayok Rd., Bungyeetho, Thunyaburi,
Pathumthani 12130 Thailand
Tel : (+66)2150-6641 (Autoline)
Email : info@p-cal.com www.p-cal.com



Calibration Report

Certificate No.: EL40429/25

Page : 3 of 3

Calibration Results

Sound Level Measurement Accuracy

(UUC Setting : A-Weighting, Time Weighting : Slow)

UUC Range	UUC Parameter	Standard Value	UUC Reading	UUC Error	Uncertainty (±)
27 to 140 dB	LFp	94 dB	94.1 dB	0.1 dB	0.17 dB
		114 dB	114.1 dB	0.1 dB	0.17 dB
27 to 140 dB	LSp	94 dB	94.1 dB	0.1 dB	0.17 dB
		114 dB	114.1 dB	0.1 dB	0.17 dB
27 to 140 dB	Llp	94 dB	94.1 dB	0.1 dB	0.17 dB
		114 dB	114.1 dB	0.1 dB	0.17 dB

(UUC Setting : A-Weighting, Time Weighting : Fast)

UUC Range	UUC Parameter	Standard Value	UUC Reading	UUC Error	Uncertainty (±)
27 to 140 dB	LFp	94 dB	94.0 dB	0.0 dB	0.17 dB
		114 dB	114.1 dB	0.1 dB	0.17 dB
27 to 140 dB	LSp	94 dB	93.9 dB	-0.1 dB	0.17 dB
		114 dB	114.1 dB	0.1 dB	0.17 dB
27 to 140 dB	Llp	94 dB	93.9 dB	-0.1 dB	0.17 dB
		114 dB	114.1 dB	0.1 dB	0.17 dB

...End...



APTITECH CALIBRATION CO., LTD.

50/40 Moo 5 T. Lat Sawai, A. Lamlukka, Pathumthani 12150
Tel. +66 2103-6290 Fax. +66 2103-6291
Email. sales@aptitech-cal.com



CERTIFICATE OF CALIBRATION

Certificate Number : EI250284

Customer : Pacific Laboratory Co.,Ltd.
Address : 14/5358 Moo 14 Tambol Bang Bua Thong Amphoe Bang Thong, Nonthaburi 11110

Description	: Sound Level Meter	W/O Number	: EI250284
Manufacturer	: Scarlet Tech	Calibration Location	: Laboratory
Model	: ST-11D	Ambient Temperature	: 22 ± 2 °C
Serial Number	: 820967	Ambient Humidity	: 55 ± 15 %RH
ID. Number	: N/A	Received Date	: 31-Jan-2025

This certifies that the above instrument was calibrated in compliance with the Calibration Systems Requirement of ISO/IEC 17025:2017 in accordance with referenced procedures. Standards used to perform this calibration are certified by or traceable to National Institute of Metrology (Thailand) and/or other recognized national measurement institutes which realizes the units of measurement according to the International System of Units (SI Unit).

Measurement uncertainties at the time of test are given where applicable. They are calculated in accordance with the method described in The Expression of Uncertainty and Confidence in Measurement (M3003).

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by coverage factor $k=2$ such that the coverage probability corresponds to approximately 95%. This result of calibration was found accurate as shown on date and place of calibration only.

Standard Equipments

Description	Serial No.	Certificate No.	Traceability	Due Date
Sound Level Calibrator	141011576	CP20240179EA	TISI: 22-LB0119	14-May-25

APTITECH

Authority of Calibration

Approved Signatory

Calibration Date : 03-Feb-2025

Issued Date : 06-Feb-2025

Calibrated By : Ms. Hathaichanok Kaewsrisai

- ☒ Mr. Anuwat Simsiriwat [Laboratory Manager]
☐ Mr. Kornupong Suksamran [Technical Manager]

Calibration certificates without signatures are not valid. This certificate applied to only the item identified and shall not be reproduced other than in full, without the specific written approval by APTITECH CALIBRATION CO., LTD.



APTITECH CALIBRATION CO., LTD.

50/40 Moo 5 T. Lat Sawai, A. Lamlukka, Pathumthani 12150
Tel. +66 2103-6290 Fax. +66 2103-6291
Email. sales@aptitech-cal.com



CALIBRATION REPORT

Certificate Number : EI250284

Calibration Method

The Unit Under Calibration (UUC) was calibrated by comparison measurement with sound level calibrator. The calibration has been accomplished in an ambient environment controlled, base on the in-house calibration procedure. The identification of the laboratory's calibration procedure employed are CP-7.2-01-107

Calibration Results

Appearance and function of use : Good
Results of Calibration : Without any adjustment
Sound Level Calibration
- Frequency Weighting : A
- Resolution : 0.1 dB

Sound Level Measurement (Slow Mode)

Parameter	UUC Range	Standard Value	UUC Reading	UUC Error	(±) Uncertainty
LFp	20-140 dB	93.86 dB	93.8 dB	-0.06 dB	0.60 dB
		113.87 dB	113.6 dB	-0.27 dB	0.60 dB
LSp	20-140 dB	93.86 dB	93.9 dB	0.04 dB	0.60 dB
		113.87 dB	113.6 dB	-0.27 dB	0.60 dB
LIp	20-140 dB	93.86 dB	93.8 dB	-0.06 dB	0.60 dB
		113.87 dB	113.5 dB	-0.37 dB	0.60 dB

Sound Level Measurement (Fast Mode)

Parameter	UUC Range	Standard Value	UUC Reading	UUC Error	(±) Uncertainty
LFp	20-140 dB	93.86 dB	93.8 dB	-0.06 dB	0.60 dB
		113.87 dB	113.7 dB	-0.17 dB	0.60 dB
LSp	20-140 dB	93.86 dB	93.8 dB	-0.06 dB	0.60 dB
		113.87 dB	113.6 dB	-0.27 dB	0.60 dB
LIp	20-140 dB	93.86 dB	93.9 dB	0.04 dB	0.60 dB
		113.87 dB	113.6 dB	-0.27 dB	0.60 dB

--- End of Certificate ---

CERTIFICATE OF CALIBRATION

NO. 20230113101

Name of Product:	Sound Level Meter
Model:	ST-11D
Serial Number:	820861
Specification:	Class 1
Conclusion:	Pass
Date of calibration:	2025-03-20
Due Date:	2026-03-20

 Calibrated by: *Jim Lin*

- I. This report certifies that all calibration equipment used in the test is traceable with the internal ISO9001 procedures and meets all specification given in the Manual(s) or respectively surpass then, and applies only to the unit identified above.
- II. This certificate is produced with advanced equipment & procedures which permit comprehensive quality assurance verification of all data supplied herein.
- III. This certificate of calibration shall not be reproduced except in full, without written permission of the Scarlet Tech Co Ltd Taiwan.

1. Preliminary inspection: OK

 2. Type & serial No. of Microphone: AWA14425-57294

 4. Measuring up limit: 140 dBA

3. Adjustments to indicated sound levels:

5. Frequency weightings (Acoustic signal tests for Z weighting, other electric signal tests.)

 Type of Calibrator B&K 4231

 Sound Pressure Level 94.0 dB

 Equivalent Free-field Sound Level (reference environment conditions) 93.8 dB

Nominal frequency /Hz	Frequency weighting / dB			Nominal frequency /Hz	Frequency weighting / dB		
	A	C	Z		A	C	Z
10	-71.0	-14.8	-0.8	1000	0.0	0.0	-0.1
20	-50.4	-6.3	-0.4	2000	1.3	-0.2	-0.1
31.5	-39.5	-3.0	-0.1	4000	1.1	-0.8	-0.1
63	-26.2	-0.8	-0.2	8000	-1.0	-3.0	0.0
125	-16.2	-0.2	-0.1	12500	-11.7	-13.7	0.0
250	-8.7	-0.1	-0.1	16000	-11.8	-13.8	0.0
500	-3.2	0.0	-0.1	20000	-23.8	-25.8	-0.3

6. Self-generated noise

Microphone replaced by electrical input signal device

10.3 dB(A)	12.2 dB(C)	19.4 dB(Z)
------------	------------	------------

7. F&S Weighting

Rate of the F weighting decrease (dB/s)	35.1
Rate of the S weighting decrease (dB/s)	4.4
Deviation of F&S	-0.1

8. Level Linearity (A-weighting at frequency 1 kHz)

Reference sound level 90.0 dB

Max error at 10dB steps upper reference sound level 0.1 dB

Max error at 1dB steps within 5dB of the upper limit linear operating range 0.0 dB

Max error at 10dB steps below reference sound level 0.1 dB

Max error at 1dB steps within 5dB upper the lower limit linear operating range 0.1 dB

9. Tone burst response (A Weighting) :

Single Toneburst duration /ms	Toneburst response /dB			
	LAFmax-LA	LASmax-LA	LAε-LA	LAeqT-LA
500	0.0	-4.0	-2.9	-7.0
200	-0.9	-7.4	-6.9	-7.0
2	-18.0	-26.9	-26.9	-7.0
0.25	-27.2	/	-36.0	-7.0

10. Peak C sound level (500Hz) :

Cycle	One cycle	nominal value	Positive half	nominal value	Negative half	nominal value
LCpeak-LC(dB)	3.5	3.5	2.3	2.4	2.3	2.4

11. Overload indication: Pass

12. Statistical analysis function

Sweep signal maximum indicated sound level: 112.8 dB

Sweep amplitude: 40 dB

Scan cycle time: 60 S; Measurement period: 180 S.

ภาคผนวกที่ 5-3
เอกสารสอบเทียบเครื่องมือตรวจวัดความสั่นสะเทือน



Metrology and Calibration Department
Electrical Maintenance Division
Electricity Generating Authority of Thailand

81 Moo 11 Bangkruai - Sainoi Rd., Sainoi, Nonthaburi 11150 Tel. (662) 436-8789 Ext. 6155



NSC-TISI-TIS 17025
CALIBRATION 0318

Certificate of Calibration

Issued by : Vibration Laboratory

Certificate No. : 25V0031

Reference No. : CBLUE01V014

Received Date : 14 March 2025

Calibrated Date : 18 March 2025

Page 1 of 3

Client : Blue Consultant Limited Partnership

Address : 32/751 Pracha - Uthit Rd., Thung Khru, Bangkok 10140

Equipment : VIBRATION METER

Manufacture /Brand : INSTANTEL

Model : Micromate

Serial No./ ID No. : UM19247

Bamrung Saengthien

(Mr. Bamrung Saengthien)

Authorized Signatory

Issue Date 18 March, 2025

This certificate is issued in accordance with the conditions of accreditation granted by The National Accreditation Council of Thailand which has assessed the measurement capability of the laboratory and its traceability to recognised national standards and to the units of measurement realised at the corresponding national standards laboratory. This certificate may not be reproduced other than in full, except with the prior written approval of the head of Calibration services and environmental analysis department. This reported measurement result relates only the measurand and applies only at the time of measurement.



Metrology and Calibration Department
Electrical Maintenance Division
Electricity Generating Authority of Thailand

Continued of Calibration Report

Certificate No. 25V0031

Page 2 of 5

Reference Standard Used

Description	Manufacture/Model	Serial No.	Traceable No.	Due Date
Accelerometer Type 8305	Brue! & Kjaer	1262817	AV-0014-23	28 March 2025
Conditioning Amplifier Type 2635	Brue! & Kjaer	2371579	AV-0013-23	27 March 2025
Digital Multimeter /8846A	FLUKE	4330020	24E513	22 September 2025

Traceability

This certificate provides traceability of measurement to the International System of Units (SI) through

- National Institute of Metrology (Thailand) (NIMT)
- Metrology and Calibration Department (EGAT)

Environmental Conditions

The calibration was performed in an environment of $(23\pm 2)^{\circ}\text{C}$ and $(50\pm 10)\%\text{RH}$

Measurement Method

The unit under calibration was calibrated by comparison with standard accelerometer. The calibration method is based on ISO 16063-21 : 2003(E) by comparison with reference accelerometer standard .

Uncertainty of Measurement

The measurement uncertainty are labeled on the following pages completed the expanded uncertainty that calculated in accordance with the method to describe in M3003, using coverage factor $k=2$, The value of the measured lies within the assigned ranges the measured lies within the assigned ranges of values to a coverage probability of approximately 95%.

Tabulation of Results

The measurement results, labeled in the following pages give the calibration results and associated measurement uncertainties.



Metrology and Calibration Department
Electrical Maintenance Division
Electricity Generating Authority of Thailand

Continued of Calibration Report

Certificate No. 25V0031

Page 3 of 3

Measurement Results

DESCRIPTION Frequency (Hz)	STD Applied Value (mm/s _p)	UUC Reading (mm/s _p)	Uncertainty (± mm/s _p)	Direction
*20	10.00	10.16	0.15	Vertical (V)
*30	10.00	10.38	0.15	
40	10.00	10.42	0.15	
80	10.00	10.41	0.15	
*20	10.00	10.27	0.15	Transverse (T)
*30	10.00	10.47	0.15	
40	10.00	10.52	0.15	
80	10.00	10.54	0.15	
*20	10.00	9.90	0.14	Longitudinal (L)
*30	10.00	9.91	0.14	
40	10.00	9.91	0.14	
80	10.00	9.88	0.14	

Note

Tranducer Part : 721A3301

Serial No. : UM19247

Remark: * Measurement results outside the scope of accreditation.

End Certificate of Calibration



CALIBRATION LABORATORY CO., LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



CERTIFICATE OF CALIBRATION

FOR

NOMENCLATURE : VIBRATION METER
MANUFACTURER : INSTANTEL
MODEL / TYPE : 721A2501/721A2901
SERIAL NO. : UM13203/UM13202
CLID. NO. : 251900155
JOB CONTROL NO. : 241221136141
CALIBRATION SERVICE : ☒ IN-LABORATORY ☐ ON-SITE

CUSTOMER : PACIFIC LABORATORY CO., LTD.
14/5358 MOO 14 TAMBOL BANG BUA THONG
AMPHOE BANG BUA THONG NONTABURI 11110

DATE OF RECEIVED : 21 December 2024

DATE OF ISSUED : 25 December 2024

The report of calibration shall not be reproduced except in full without approval of the Calibration Laboratory Co., Ltd.

Calibrated By : Suwit Phuanbusabong
Calibration Engineer



Approved By : Mongkol Yotsoontorn
Authorized Signatory
25 December 2024

This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to the
International System of Units (SI)

Certificate No. Q24136141

F3-011-05/12-23



@clccalibration



CALIBRATION LABORATORY CO., LTD.

2/10-11,14, 55 Soi Prasert Manukil 29 Yaek 4, Prasert Manukil Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



REPORT OF CALIBRATION FOR

NOMENCLATURE	:	VIBRATION METER
MANUFACTURER	:	INSTANTEL
MODEL / TYPE	:	721A2501/721A2901
SERIAL NO.	:	UM13203/UM13202
DATE OF CALIBRATION	:	23 December 2024

ENVIRONMENT CONDITIONS :

Temperature : $(23 \pm 2) ^\circ\text{C}$

Relative Humidity : $(55 \pm 15) \% \text{RH}$

PROCEDURE USED :

This instrument was calibrated under procedure No. **CLC-CPEE-08** based on **ISO 16063-21** as calibration guideline.
The calibration was performed by using Digital Multimeter, Programmable Timer/Counter, Vibration Calibrator which maintained by the Calibration Laboratory Co., Ltd.

REFERENCE STANDARD USED :

1. Vibration Calibrator, The Modal Shop Model 9110D S/N. 11424.
2. Programmable Timer/Counter, Philips Model PM6680B S/N. SM607101.
3. Digital Multimeter, Keysight Technologies Model 3458A S/N. MY59352733.

TRACEABILITY :

1. The measurements are traceable to International System of Units (SI), through National Institute of Metrology (Thailand) Certificate No. AV-0030-24, Due Date 19 July 2025.
2. The measurements are traceable to International System of Units (SI), through Aeronautical Radio of Thailand Ltd. Certificate No. 07-0050/24 , Due Date 13 May 2025 .
3. The measurements are traceable to International System of Units (SI), through National Institute of Metrology (Thailand) Certificate No. EE-0060-24, Due Date 26 June 2025.

UNCERTAINTY :

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor $k = 2,00$ which for a normal distribution corresponds to a coverage probability of approximately 95 %.
It has been evaluated according to the "Evaluation of the Uncertainty of Measurement in Calibration (EA-4/02 M:2022)"

Certificate No. **Q24136141**

F3-011-05/12-23

page 2 of 3



@clccalibration



CALIBRATION LABORATORY CO., LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel: 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



CONDITION OF CALIBRATION ITEM : RECEIVED IN GOOD OPERATIONAL CONDITION

MEASUREMENT RESULTS : (X) without adjustment () adjustment

CALIBRATION DATA

VELOCITY RESULT

Test point		Mode	STD Reading	DUC Reading	Correction	Uncertainty
(mm/s)	(frequency)		(mm/s)	(mm/s)	(mm/s)	\pm (% of rdg.)
10	160 Hz	peak	10.000	10.342	-0.342	1.5
20	160 Hz		20.000	20.414	-0.414	1.5
30	160 Hz		30.000	30.497	-0.497	1.5
40	160 Hz		40.000	40.595	-0.595	1.5
50	160 Hz		50.000	50.717	-0.717	1.5

Note. The Scope of Accredited ANAB Certificate No. ACDM-2814 Version 012 Page 2 of 67

This report is valid for the above stated instrument/s only.

End of Certificate

Certificate No. Q24136141

F3-011-05/12-23

page 3 of 3



@clccalibration



CALIBRATION LABORATORY Co., LTD.

2/10-11, 14, 55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail: sale@cal-laboratory.com



CERTIFICATE OF CALIBRATION

FOR

NOMENCLATURE : VIBRATION METER
MANUFACTURER : INSTANTEL
MODEL / TYPE : 721A2501/721A2901
SERIAL NO. : UM13202/UM13202
CLID. NO. : 252102517
JOB CONTROL NO. : 241219135224
CALIBRATION SERVICE : ☒ IN-LABORATORY ☐ ON-SITE

CUSTOMER : PACIFIC LABORATORY CO., LTD.
14/5358 MOO 14 TAMBOL BANG BUA THONG
AMPHOE BANG BUA THONG NONTABURI 11110

DATE OF RECEIVED : 19 December 2024

DATE OF ISSUED : 23 December 2024

The report of calibration shall not be reproduced except in full without approval of the Calibration Laboratory Co., Ltd.

Calibrated By :

Suwit Phuanbusabong
Calibration Engineer



Approved By :

Mongkol Yotsoontorn
Authorized Signatory
23 December 2024

This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to the
International System of Units (SI)

Certificate No. Q24135224

F3-011-05/12-23



@clccalibration



CALIBRATION LABORATORY CO., LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



REPORT OF CALIBRATION FOR

NOMENCLATURE	:	VIBRATION METER
MANUFACTURER	:	INSTANTEL
MODEL / TYPE	:	721A2501/721A2901
SERIAL NO.	:	UM13202/UM13202
DATE OF CALIBRATION	:	20 December 2024

ENVIRONMENT CONDITIONS :

Temperature : $(23 \pm 2) ^\circ\text{C}$

Relative Humidity : $(55 \pm 15) \% \text{RH}$

PROCEDURE USED :

This instrument was calibrated under procedure No. CLC-CPEE-08 based on ISO 16063-21 as calibration guideline.

The calibration was performed by using Digital Multimeter, Programmable Timer/Counter, Vibration Calibrator which maintained by the Calibration Laboratory Co., Ltd.

REFERENCE STANDARD USED :

1. Vibration Calibrator, The Modal Shop Model 9110D S/N. 11424.
2. Programmable Timer/Counter, Philips Model PM6680B S/N. SM607101.
3. Digital Multimeter, Keysight Technologies Model 3458A S/N. MY59352733.

TRACEABILITY :

1. The measurements are traceable to International System of Units (SI), through National Institute of Metrology (Thailand) Certificate No. AV-0030-24, Due Date 19 July 2025.
2. The measurements are traceable to International System of Units (SI), through Aeronautical Radio of Thailand Ltd. Certificate No. 07-0050/24, Due Date 13 May 2025.
3. The measurements are traceable to International System of Units (SI), through National Institute of Metrology (Thailand) Certificate No. EE-0060-24, Due Date 26 June 2025.

UNCERTAINTY :

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor $k = 2,00$ which for a normal distribution corresponds to a coverage probability of approximately 95 %. It has been evaluated according to the "Evaluation of the Uncertainty of Measurement in Calibration (EA-4/02 M:2022)"

Certificate No. Q24135224

F3-011-05/12-23

page 2 of 3



@clccalibration



CALIBRATION LABORATORY Co., LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



CONDITION OF CALIBRATION ITEM : RECEIVED IN GOOD OPERATIONAL CONDITION

MEASUREMENT RESULTS : (X) without adjustment () adjustment

CALIBRATION DATA

VELOCITY RESULT

Test point		Mode	STD Reading	DUC Reading	Correction	Uncertainty
(mm/s)	(frequency)		(mm/s)	(mm/s)	(mm/s)	\pm (% of rdg.)
10	160 Hz	peak	10.000	10.324	-0.324	1.5
20	160 Hz		20.000	20.388	-0.388	1.5
30	160 Hz		30.000	30.465	-0.465	1.5
40	160 Hz		40.000	40.572	-0.572	1.5
50	160 Hz		50.000	50.689	-0.689	1.5

Note. The Scope of Accredited ANAB Certificate No. ACDM-2814 Version 012 Page 2 of 67

This report is valid for the above stated instrument/s only.

End of Certificate

Certificate No. Q24135224

F3-011-05/12-23

page 3 of 3



@clccalibration



Metrology and Calibration Department
Electrical Maintenance Division
Electricity Generating Authority of Thailand

81 Moo 11 Bangkrui - Sainoi Rd., Sainoi, Nonthaburi 11150 Tel. (662) 436-8789 Ext. 6155



NSC-TISI-TIS 17025
CALIBRATION 0318

Certificate of Calibration

Issued by : Vibration Laboratory

Certificate No. : 25V0033

Reference No. : CBLUE01V016

Received Date : 14 March 2025

Calibrated Date : 20 March 2025

Page 1 of 3

Client : Blue Consultant Limited Partnership

Address : 32/751 Pracha-uthit Rd.
Thungkhru Bangkok 10140

Equipment : VIBRATION METER

Manufacture /Brand : INSTANTEL

Model : Micromate

Serial No./ ID No. : UM8882

(Mr. Bamrung Saengthien)

Authorized Signatory

Issue Date 21 / March / 2025

This certificate is issued in accordance with the conditions of accreditation granted by The National Accreditation Council of Thailand which has assessed the measurement capability of the laboratory and its traceability to recognised national standards and to the units of measurement realised at the corresponding national standards laboratory. This certificate may not be reproduced other than in full, except with the prior written approval of the head of Calibration services and environmental analysis department. This reported measurement result relates only the measurand and applies only at the time of measurement.

FM-02/QP-MCC-09 Rev.5

e-mail : MCC@egat.co.th



Metrology and Calibration Department
Electrical Maintenance Division
Electricity Generating Authority of Thailand

Continued of Calibration Report

Certificate No. 25V0033

Page 2 of 3

Reference Standard Used

Description	Manufacture/Model	Serial No.	Traceable No.	Due Date
Accelerometer Type 8305	Brue! & Kjaer	1262817	AV-0014-23	28 March 2025
Conditioning Amplifier Type 2635	Brue! & Kjaer	2371579	AV-0013-23	27 March 2025
Digital Multimeter /8846A	FLUKE	4330020	24E513	22 September 2025

Traceability

This certificate provides traceability of measurement to the International System of Units (SI) through

- National Institute of Metrology (Thailand) (NIMT)
- Metrology and Calibration Department (EGAT)

Environmental Conditions

The calibration was performed in an environment of $(23\pm 2)^{\circ}\text{C}$ and $(50\pm 10)\%\text{RH}$

Measurement Method

The unit under calibration was calibrated by comparison with standard accelerometer. The calibration method is based on ISO 16063-21 : 2003(E) by comparison with reference accelerometer standard .

Uncertainty of Measurement

The measurement uncertainty are labeled on the following pages completed the expanded uncertainty that calculated in accordance with the method to describe in M3003, using coverage factor $k=2$, The value of the measured lies within the assigned ranges the measured lies within the assigned ranges of values to a coverage probability of approximately 95%.

Tabulation of Results

The measurement results, labeled in the following pages give the calibration results and associated measurement uncertainties.



Metrology and Calibration Department
Electrical Maintenance Division
Electricity Generating Authority of Thailand

Continued of Calibration Report

Certificate No. 25V0033

Page 3 of 3

Measurement Results

DESCRIPTION Frequency (Hz)	STD Applied Value (mm/s _p)	UUC Reading (mm/s _p)	Uncertainty (± mm/s _p)	Direction
*20	10.00	10.39	0.15	Vertical (V)
*30	10.00	10.31	0.15	
40	10.00	10.20	0.15	
52	10.00	10.12	0.15	
63	10.00	10.07	0.15	
80	10.00	10.00	0.15	
*20	10.00	10.29	0.15	Transverse (T)
*30	10.00	10.32	0.15	
40	10.00	10.30	0.15	
52	10.00	10.26	0.15	
63	10.00	10.24	0.15	
80	10.00	10.21	0.15	
*20	10.00	10.29	0.15	Longitudinal (L)
*30	10.00	10.34	0.15	
40	10.00	10.33	0.15	
52	10.00	10.29	0.15	
63	10.00	10.28	0.15	
80	10.00	10.25	0.15	

Note

Tranducer Part : ENAB16145

Serial No. : -

Remark: * Measurement results outside the scope of accreditation.

End Certificate of Calibration

ภาคผนวกที่ 5-4
เอกสารสอบเทียบเครื่องมือตรวจวัดคุณภาพน้ำ

CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhprachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech.cal@yahoo.com, calibratech.cal@hotmail.com



NSC-TISI-TIS 17025
CALIBRATION 0030

Certificate of Calibration

Certificate No. : 67-420078-1 **Page : 1 of 2**

Submitted by : Pacific Laboratory Co., Ltd.
14/5358 Moo 14, T. Bang Bua Thong, A. Bang Bua Thong, Nonthaburi 11110 Thailand

Equipment : pH Meter with electrode
pH meter
Manufacturer : Eutech Model : pH 700
Range : N/A pH Resolution : 0.01 pH
Serial No. : 2841305 ID No. : LAB-PH-002
Electrode
Model : N/A Serial No. : 3172493

Environment : On site calibration was carried out at the Laboratory, Pacific Laboratory Co., Ltd.
Ambient Temperature : (25.0 to 26.0)^o C
Relative Humidity : (40 to 45) %

Date of Received : 30 July 2024
Date of Calibration : 30 July 2024
Date of Issue : 03 August 2024
Calibrated by : Permpoon Chanpu

Calibration Method : In-house method CAL-M4201 direct measurement by using standard voltage calibrator and using certified reference material (CRM)


Reference Standard Instruments : This certification is traceable to the International System of Units

1. Multiproduct Calibrator

ID No.	Cert. No.	Due Date	Traceability
400005	SG-E-00307/66	23 Aug 2025	National Institute of Metrology Thailand (NIMT)

2. Standard Buffer Solution

pH	Cert. No.	Lot No.	Exp. Date	Traceability
4.008	61293328	986281	25 Apr 2026	CPA Chem Ltd. Accredited to ISO 17034 and ISO/IEC 17025
6.986	61281486	986283	25 Apr 2025	CPA Chem Ltd. Accredited to ISO 17034 and ISO/IEC 17025
9.997	61281073	986282	25 Apr 2025	CPA Chem Ltd. Accredited to ISO 17034 and ISO/IEC 17025

Approved by : 
(Surachai Promthong)
Laboratory Manager

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.

CAL-F0031-03



CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhaprachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech.cal@yahoo.com, calibratech.cal@hotmail.com

Certificate of Calibration

Certificate No. : 67-420078-1

Page : 2 of 2

Result of Calibration :

UUC Condition As-Received : Good

Function : Electrical measurement

pH meter

Performing standard curve by Multiproduct Calibrator at pH (4,7,10)

Adjustment Curve at nominal pH	Applied Voltage (mV)	Nominal Value (pH)	UUC Reading		Correction (mV)	Uncertainty (± mV)
			(pH)	(mV)		
4, 7, 10	177.4800	4	4.00	177.5	0.0	0.12
	0.0000	7	7.00	0.1	-0.1	0.086
	-177.4800	10	10.00	-177.4	-0.1	0.12

Function : pH meter with electrode

Performing a three - buffer standard curve using buffer nominal pH (4,7,10)

Adjustment Curve at nominal pH	Standard Buffer (pH)	UUC Reading (pH)	Correction (pH)	Uncertainty (± pH)
4, 7, 10	4.008	4.01	0.00	0.0097
	6.986	7.00	-0.01	0.011
	9.997	10.01	-0.01	0.014

Remark

UUC : Unit Under Calibration

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurment was based on a standard uncertainty multiplied by a coverage factor $k = 2$,
providing a level of confidence of approximately 95%

- 000 -



CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhprachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech.cal@yahoo.com, calibratech.cal@hotmail.com



Certificate of Calibration

Certificate No. : 67-420078-2

Page : 1 of 2

Submitted by : Pacific Laboratory Co., Ltd.

14/5358 Moo 14, T. Bang Bua Thong, A. Bang Bua Thong, Nonthaburi 11110 Thailand

Equipment : pH Meter with electrode

pH meter

Manufacturer : Eutech

Model : pH 700

Range : N/A

pH

Resolution : 0.01 pH

Serial No. : 2841305

ID No. : LAB-PH-002

Electrode

Model : N/A

Serial No. : 3052953

Environment : On site calibration was carried out at the Laboratory, Pacific Laboratory Co., Ltd

Ambient Temperature : (25.0 to 26.0)^o C

Relative Humidity : (40 to 45) %

Date of Received : 30 July 2024

Date of Calibration : 30 July 2024

Date of Issue : 03 August 2024

Calibrated by : Permpoon Chanpu

Calibration Method : In-house method CAL-M4201 direct measurement by using standard voltage calibrator and using certified reference material (CRM)

Reference Standard Instruments : This certification is traceable to the International System of Units

1. Multiproduct Calibrator

ID No.	Cert. No.	Due Date	Traceability
400005	SG-E-00307/66	23 Aug 2025	National Institute of Metrology Thailand (NIMT)

2. Standard Buffer Solution

pH	Cert. No.	Lot No.	Exp. Date	Traceability
4.008	61293328	986281	25 Apr 2026	CPA Chem Ltd. Accredited to ISO 17034 and ISO/IEC 17025
6.986	61281486	986283	25 Apr 2025	CPA Chem Ltd. Accredited to ISO 17034 and ISO/IEC 17025
9.997	61281073	986282	25 Apr 2025	CPA Chem Ltd. Accredited to ISO 17034 and ISO/IEC 17025

Approved by :

(Surachai Promthong)

Laboratory Manager

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhprachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech.cal@yahoo.com, calibratech.cal@hotmail.com

Certificate of Calibration

Certificate No. : 67-420078-2

Page : 2 of 2

Result of Calibration :

UUC Condition As-Received : Good

Function : Electrical measurement

pH meter

Performing standard curve by Multiproduct Calibrator at pH (4,7,10)

Adjustment Curve at nominal pH	Applied Voltage (mV)	Nominal Value (pH)	UUC Reading		Correction (mV)	Uncertainty (± mV)
			(pH)	(mV)		
4, 7, 10	177.4800	4	4.00	177.5	0.0	0.12
	0.0000	7	7.00	0.1	-0.1	0.086
	-177.4800	10	10.00	-177.4	-0.1	0.12

Function : pH meter with electrode

Performing a three - buffer standard curve using buffer nominal pH (4,7,10)

Adjustment Curve at nominal pH	Standard Buffer (pH)	UUC Reading (pH)	Correction (pH)	Uncertainty (± pH)
4, 7, 10	4.008	4.01	0.00	0.0097
	6.986	7.00	-0.01	0.011
	9.997	10.01	-0.01	0.014

Remark

UUC : Unit Under Calibration

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

- o0o -



CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhprachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech.cal@yahoo.com, calibratech.cal@hotmail.com



NSC-TISI-TIS17025
CALIBRATION 0030

Certificate of Calibration

Certificate No. : 67-400424-1

Page : 1 of 2

Submitted by : Pacific Laboratory Co., Ltd
14/5358 Moo 14, T. Bang Bua Thong, A. Bang Bua Thong, Nonthaburi 11110 Thailand

Equipment : Digital Thermometer with Thermistor probe
Temperature Indicator

Manufacturer : Eutech Model : pH 700
Range : N/A °C Resolution : 0.1 °C
Serial No. : 2841305 ID No. : LAB-PH-002
Thermistor probe

Model : N/A Sheath Material : Stainless
Diameter : 3 mm. Length : 115 mm.
Serial No. : PHSTEMB01P 304 ID No. : LAB-PH-002

Environment : On site calibration was carried out at the Laboratory, Pacific Laboratory Co., Ltd

Ambient Temperature : (25.0 to 25.6) °C
Relative Humidity : (45 to 47) %
Line Voltage : (220.0 to 222.0) VAC

Date of Received : 30 July 2024

Date of Calibration : 30 July 2024

Date of Issue : 03 August 2024

Calibrated by : Permpon Chanpu

Calibration Method : This instrument was calibrated by In-house method comparison technique CAL-M4003 by compared with PRT in the liquid bath at the constant controlled temperature.

The temperature scale used was based on ITS-90

Reference Standard Instruments : This certification is traceable to the International System of Units

1. Platinum Resistance Thermometer (PRT)

ID No.	Cert. No.	Due Date	Traceability
400002	TT-0074-22	23 Aug 2025	National Institute of Metrology Thailand (NIMT)

2. Standard Digital Thermometer

ID No.	Cert. No.	Due Date	Traceability
400033	22E569	25 Apr 2025	National Institute of Metrology Thailand (NIMT)

Approved by :

(Bunjerd Masri)

Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhprachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech.cal@yahoo.com, calibratech.cal@hotmail.com

Certificate of Calibration

Certificate No. : 67-400424-1

Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Function : Temperature measurement

Immersion Depth (mm.)	Standard Reading (°C)	UUC Reading (°C)	Correction (°C)	Uncertainty (± °C)
115	25.005	24.8	0.2	0.19

Remark

UUC : Unit Under Calibration

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

- ๐() ๐ -

B/



CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhaprachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech.cal@yahoo.com, calibratech.cal@hotmail.com



NSC-TISI-TIS 17025
CALIBRATION 0030

Certificate of Calibration

Certificate No. : 67-400454-3

Page : 1 of 2

Submitted by : Pacific Laboratory Co., Ltd
14/5358 Moo 14, T. Bang Bua Thong, A. Bang Bua Thong, Nonthaburi 11110 Thailand

Equipment : Temperature controlled enclosure (Incubator)
Manufacturer : Aqua Lytic Model : TC 135S
Range : N/A °C Resolution : 0.1 °C
Serial No. : 0614/000033 ID No. : LAB-IB-001

Environment : On site calibration was carried out at the Laboratory, Pacific Laboratory Co., Ltd
Ambient Temperature : (25.5 to 26.0) °C
Relative Humidity : (40 to 45) %
Line Voltage : (220.0 to 222.0) V

Date of Received : 30 July 2024

Date of Calibration : 30 July 2024

Date of Issue : 03 August 2024

Calibrated by : Permpoon Chanpu

Calibration Method : CAL-M4004, TLAS G-20

The temperature scale used was based on ITS-90

Reference Standard Instruments : This certification is traceable to the International System of Units
Standard Digital Thermometer with RTD Probe

<u>ID No.</u>	<u>Cert. No.</u>	<u>Due Date</u>	<u>Traceability</u>
400029 & 400043	67-400245-1	27 Oct 2024	National Institute of Metrology Thailand (NIMT)

Approved by :

(Surachai Promthong)

Laboratory Manager

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhaphrachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech.cal@yahoo.com, calibratech.cal@hotmail.com

Certificate of Calibration

Certificate No. : 67-400454-3


Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Function : Temperature measurement

This instrument was setting air ventilation at position 0 (close)

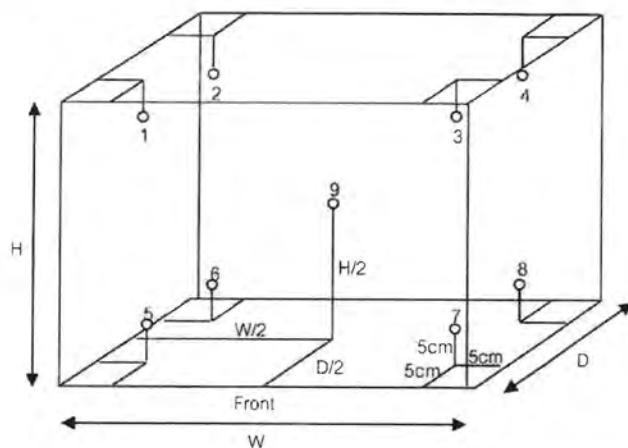

Inside of Chamber

W = 0.51 m

D = 0.04 m

H = 0.70 m

Capacity = 0.02 m³

Test Point (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Temperature (°C) @ Sensor No.									Uncertainty (± °C)
			1	2	3	4	5	6	7	8	9	
20.0	20.5	20.5	20.07	19.92	19.95	19.93	19.93	19.92	19.92	19.96	19.88	0.67

Test Point (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Uniformity (°C)	Measured Stability (°C)	Overall Variation (°C)
20.0	20.5	20.5	0.41	0.33	0.70

Remark The uncertainty is not combine uniformity of the air chamber

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

- o0o -



CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhaphrachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech.cal@yahoo.com, calibratech.cal@hotmail.com



Certificate of Calibration

Certificate No. : 67-400454-2

Page : 1 of 2

Submitted by : Pacific Laboratory Co., Ltd

14/5358 Moo 14, T. Bang Bua Thong, A. Bang Bua Thong, Nonthaburi 11110 Thailand

Equipment : Water Bath

Manufacturer : Memmert

Model : WNB 22

Range : N/A °C

Resolution : 0.1 °C

Serial No. : L514.0184

ID No. : LAB-WB-001

Environment : On site calibration was carried out at the Laboratory, Pacific Laboratory Co., Ltd

Ambient Temperature : (30.0 to 31.3) °C

Relative Humidity : (60 to 65) %

Line Voltage : (220.0 to 222.0) V

Date of Received : 30 July 2024

Date of Calibration : 30 July 2024

Date of Issue : 03 August 2024

Calibrated by : Permpon Chanpu

Calibration Method : This instrument was calibrated by In-house method CAL-M4006 based on ASTM E715-80
The temperature scale used was based on ITS-90

Reference Standard Instruments : This certification is traceable to the International System of Units

Standard Digital Thermometer with RTD probe

ID No.

Cert. No.

Due Date

Traceability

400029 & 400031 67-400244-1

24 Oct 2024

National Institute of Metrology Thailand (NIMT)

Approved by :

(Surachai Promthong)

Laboratory Manager

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhaphrachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech.cal@yahoo.com, calibratech.cal@hotmail.com

Certificate of Calibration


Certificate No. : 67-400454-2

Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Function : Temperature measurement

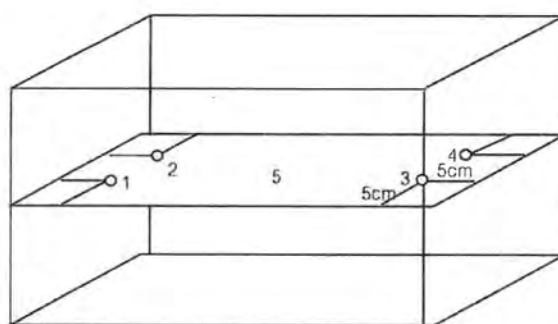

Front

Test Point (" C)	Setting Temperature (" C)	Indicating Temperature (" C)	Measured Temperature (" C) @ Sensor					Uncertainty (± " C)	Measured Uniformity (" C)	Measured Stability (" C)
			No.							
			1	2	3	4	5			
65.0	65.0	65.0	64.61	64.70	64.66	64.64	64.68	0.18	0.12	0.05
95.0	95.0	95.0	94.60	94.69	94.70	94.61	94.70	0.18	0.15	0.03

Remark The uncertainty is not combine uniformity of the water bath

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

- o0o -

ABJ



CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhprachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech.cal@yahoo.com, calibratech.cal@hotmail.com



NSC-TISI-TIS17025
CALIBRATION 0030

Certificate of Calibration

Certificate No. : 67-400454-1

Page : 1 of 2

Submitted by : Pacific Laboratory Co., Ltd
14/5358 Moo 14, T. Bang Bua Thong, A. Bang Bua Thong, Nonthaburi 11110 Thailand

Equipment : Temperature controlled enclosure (Oven)
Manufacturer : Memmert Model : UN 55
Range : N/A °C Resolution : 0.1 °C
Serial No. : B214.1879 ID No. : LAB-OV-001

Environment : On site calibration was carried out at the Laboratory, Pacific Laboratory Co., Ltd
Ambient Temperature : (30.0 to 31.3) °C
Relative Humidity : (60 to 65) %
Line Voltage : (220.0 to 222.0) V

Date of Received : 30 July 2024

Date of Calibration : 30 July 2024

Date of Issue : 03 August 2024

Calibrated by : Permpon Chanpu

Calibration Method : CAL-M4Q04, TLAS G-20

The temperature scale used was based on ITS-90

Reference Standard Instruments : This certification is traceable to the International System of Units
Standard Digital Thermometer with Thermocouple probe

<u>ID No.</u>	<u>Cert. No.</u>	<u>Due Date</u>	<u>Traceability</u>
400029 & 400030	67-400246-1	25 Oct 2024	National Institute of Metrology Thailand (NIMT)

Approved by :

(Surachai Promthong)

Laboratory Manager

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhaphrachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech.cal@yahoo.com, calibratech.cal@hotmail.com

Certificate of Calibration

Certificate No. : 67-400454-1


Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Function : Temperature measurement

This instrument was setting air ventilation at position 0 (close)

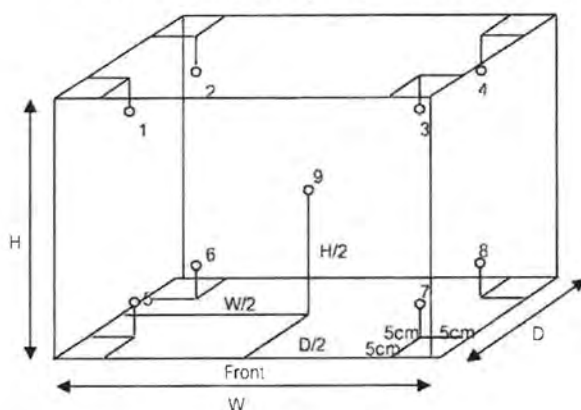

Inside of Chamber

W = 0.40 m

D = 0.33 m

H = 0.40 m

Capacity = 0.05 m³

Test Point (° C)	Setting Temperature (° C)	Indicating Temperature (° C)	Measured Temperature (° C) @ Sensor No.									Uncertainty
			1	2	3	4	5	6	7	8	9	(± ° C)
104.0	107.0	107.0	105.1	104.9	104.8	104.8	102.9	103.6	103.7	104.1	103.9	0.84
180.0	184.0	184.0	180.5	180.5	180.3	179.7	176.8	177.2	178.1	181.2	179.5	1.4

Test Point (° C)	Setting Temperature (° C)	Indicating Temperature (° C)	Measured Uniformity (° C)	Measured Stability (° C)	Overall Variation (° C)
104.0	107.0	107.0	1.4	0.4	2.5
180.0	184.0	184.0	3.3	0.7	5.6

Remark The uncertainty is not combine uniformity of the air chamber

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

- o0o -



Calibration Certificate

Certificate No.: 2502229-006-01
Client name: UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.
Address: 3 Soi Udomsuk 41, Sukhumvit Road,
Bangchack, Prakhonong, Bangkok 10260

Page 1 of 3

Equipment: CHAMBER (Incubator)

Manufacturer: BINDER

Model: KB 400

Serial No.: 20200000015535

ID No.: UAE.MIC.018/2564


Order No.: 2502229

Operation No.: 2502229-006

Date of Receipt: 19 March 2025

Date of Calibration: 19 March 2025

Calibrated by Mr.Jerawut Prapawuttipong
Scientist

Approved by 
(Mr.Pheraphat Tuanjit) (for)
Manager, Division of Calibration Laboratory
Responsible for the Technical Management Team

Date of Issue: 25 March 2025

The uncertainties are for a confidence probability of approximately 95 %.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the National Food Institute.

F-CS-009 Revision: 01 Date: 20-04-65

กรมอุตสาหกรรม
จังหวัดนนทบุรี

List Certificate of Laboratory Instrument

No. Instrument/Equipment	Parameter	Manufacturer	Model/Serial No.	Calibrator	Certification No.	Date of Calibration	Due date of Calibration*	Remark
Laboratory Instrument for Water Quality Analysis								
1	Incubator	Binder	KB400 / 20200000015535	National Food Institute, Ministry of Industry, Thailand	2502229-006-01	19 Mar 25	18 Mar 26	
2	Incubator		B 75 / 101170001	National Food Institute, Ministry of Industry, Thailand	2502229-004-01	25 Mar 25	19 Mar 26	
3	Incubator		B 75 / 101170007	National Food Institute, Ministry of Industry, Thailand	2502229-005-01	20 Mar 25	19 Mar 26	
4	Incubator		B 75 / 101170007	National Food Institute, Ministry of Industry, Thailand	2502229-001-01	19 Mar 25	18 Mar 26	
5	Water Bath		WAE 18 / 14112452	Technology Promotion Association (Thailand-Support)	2574501	19 Mar 25	18 Mar 26	
6	Water Bath		WAE 18 / 14112452	Technology Promotion Association (Thailand-Support)	2574503	19 Mar 25	18 Mar 26	
7	Analytical Balance		PH203 / 0256754150	National Food Institute, Ministry of Industry, Thailand	2502229-000-01	19 Mar 25	18 Mar 26	
8	Auto Clave	ACP	15-400 / 808763	National Food Institute, Ministry of Industry, Thailand	2502229-007-01	19 Mar 25	18 Mar 26	

Due Date of Calibration*: Based on the annual calibration plan. At least 1 time per year.

เอกสารไม่ควบคุม

1/1

วันที่ 19 มีนาคม 2565
ห้องปฏิบัติการมาตรฐาน ISO/IEC 17025

เอกสารไม่ควบคุม



nfi-th



สถาบันพัฒนาบุคลากรด้านอาหาร
ศูนย์บริการห้องปฏิบัติการอุตสาหกรรมอาหาร
Foundation for Industrial Development National Food Institute
Food Industrial Laboratory Service Center



Calibration Report

Certificate No.: 2502229-006-01
Equipment: CHAMBER (Incubator)
Model: KB 400 Serial No.: 20200000015535
Resolution: 0.1 °C ID No.: UAE-MIC.018/2564
Manufacturer: BINDER
Date of Calibration: 19 March 2025

Page 2 of 3

Location: LABORATORY, UNITED ANALYST AND ENGINEERING CONSULTANT CO., LTD.
Environment Condition: Ambient Temperature (18 ± 1) °C
Relative Humidity (50 ± 5) %
Line Voltage (223 ± 3) Volt

Condition of this results of Calibration:

- This instrument was calibrated by insert 13 standard thermometer into its chamber and calibration according to W-TE-014 Based on TLAS G-20-1/02-08 (E); Guidelines for Calibration and Checks of Temperature Controlled Enclosures.
- The temperature scale used was based on ITS - 90.
- All data show below were final values and the initial data may be obtained upon request.

2. Reference Standard Instrument :

Instrument	Model	Serial No./ID No.	Certificate No.	Due Date	Through
Digital Thermometer with sensor	34972A RTD	MY49016851 CHP201-303 / RTD#201-303	TE 670477-01	4 May 2025	NATIONAL FOOD INSTITUTE

- This certificate is traceable to International System of Units (SI Units).
- This certificate was certified only for the instrument we calibrated.
- This result of calibration was found accurate as shown on date and place of calibration only.
- Condition of Calibrated item : Good

UUC Description :

Time of Record : 1 Hour 9 Minute At : 35.0 °C
Fresh air Damper : ☒ Open Position ☒ Close Fan ☒ Not Available

7. Result of Calibration : ☒ Without adjustment ☐ After adjustment

P. Jongsakul
25 March 2025

FCS-012 Revision: 01 Date: 20-04-65

2008 ถนนสุขุมวิท 36 แขวงคลองเตย เขตคลองเตย กรุงเทพมหานคร 10110
2008 Soi 36, Asoke Areea Road, Bang Yi Khan Subdistrict, Bang Phae District, Bangkok 10710, Thailand
Tel: +66(0) 2422 8628 Fax: +66(0) 2422 8545



สถาบันพัฒนาบุคลากรด้านอาหาร
ศูนย์บริการห้องปฏิบัติการอุตสาหกรรมอาหาร
Foundation for Industrial Development National Food Institute
Food Industrial Laboratory Service Center



Calibration Report

Certificate No.: 2502229-006-01
Equipment: CHAMBER (Incubator)
Model: KB 400 Serial No.: 20200000015535
Resolution: 0.1 °C ID No.: UAE-MIC.018/2564
Manufacturer: BINDER
Date of Calibration: 19 March 2025

Page 3 of 3

Calibration point: 35.0 °C

Calibration result:

Calibration Condition	Temperature (°C)	Relative Humidity (%)	Line Voltage (Volt)
MIN	17.1	45	220.0
MAX	18.1	55	225.0

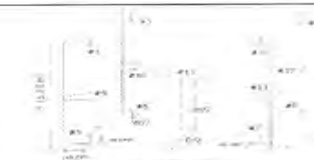


Table1 : Reporting of Temperature

Calibration point (°C)	Measured Temperature (°C) @ Sensor No. (Sensor No.13 is REF)													Uncertainty ± (°C)
	# 1	# 2	# 3	# 4	# 5	# 6	# 7	# 8	# 9	# 10	# 11	# 12	# 13	
35.0	34.98	35.17	34.99	34.92	35.18	35.01	35.00	35.13	35.00	34.96	35.02	35.17	35.04	0.27

Table 2 : Reporting of Characterization Result

UUC* Setting (°C)	UUC* Reading (°C)			Temperature Stability ± (°C)	Temperature Uniformity (°C)	Overall Variation (°C)
	MIN	MAX	Average			
35.0	35.0	35.0	35.0	0.029	0.15	0.30

Note : The quoted uncertainty include " Stability " and " Loading effect (20% of Temp Uniformity) "

UUC* = Unit Under Calibration

Stability = One-half of the greatest maximum difference of measured temperatures at any one sensors, for at least half an hour after reaching steady state.

Uniformity = The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time.

Overall Variation = The difference of the maximum and minimum measured temperatures throughout observation time.

The report uncertainty of measurement was based on standard uncertainty multiplied by coverage factor k= 2, providing a level of confidence of approximately 95 %.

----- End -----

P. Jongsakul
25 March 2025

FCS-012 Revision: 01 Date: 20-04-65

2008 ถนนสุขุมวิท 36 แขวงคลองเตย เขตคลองเตย กรุงเทพมหานคร 10110
2008 Soi 36, Asoke Areea Road, Bang Yi Khan Subdistrict, Bang Phae District, Bangkok 10710, Thailand
Tel: +66(0) 2422 8628 Fax: +66(0) 2422 8545



Calibration Certificate

Certificate No.: 2502229-004-01
Client name: UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.
Address: 3 Soi Udomsuk 41, Sukhumvit Road,
 Bangchack, Prakhnong, Bangkok 10260

Page 1 of 3

Equipment:	CHAMBER (Incubator)
Manufacturer:	MEMMERT
Model:	IN75
Serial No.:	D317.0305
ID No.:	UAE.MTC.022/2561
Order No.:	2502229
Operation No.:	2502229-004
Date of Receipt:	19 March 2025
Date of Calibration:	20 March 2025

Calibrated by Mr.Yothin Charoensuk
Scientist

Approved by

P. Jenghachit
(Mr. Pheraphat Tuanjit) (for)

Manager, Division of Calibration Laboratory

Responsible for the Technical Management Team

Date of Issue: 25 March 2025

The uncertainties are for a confidence probability of approximately 95 %.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the National Food Institute.

F-CS-009 Revision: 01 Date: 20-04-65

Calibration Report

Certificate No.: 2502229-004-01

Equipment: CHAMBER (Incubator)

Model: IN75 **Serial No.:** D317.0305

Resolution: 0.1 °C **ID No.:** UAE.MIC.022/2561

Manufacturer: MEMMERT

Date of Calibration: 20 March 2025

Page 2 of 3

Location: 302, UNITED ANALYST AND ENGINEERING CONSULTANT CO., LTD.

Environment Condition:

Ambient Temperature	(28.8 ± 1) °C
Relative Humidity	(59 ± 1) %
Line Voltage	(223 ± 3) Volt

Condition of this results of Calibration:

1. This instrument was calibrated by insert 9 standard thermometer into its chamber and calibration according to W-TE-014 Based on TLAS G-20-1/02-08 (E): Guidelines for Calibration and Checks of Temperature Controlled Enclosures.
- The temperature scale used was based on ITS - 90.
 - All data show below were final values and the initial data may be obtained upon request.

Instrument	Model	Serial No./ID No.	Certificate No.	Due Date	Through
Digital Thermometer with sensor	34972A	MYS7003188	TE 670486-01	8 June 2025	NATIONAL FOOD INSTITUTE
	RTD	CH#101-109/RTD#101-109			

3. This certificate is traceable to International System of Units (SI Units).
4. This certificate was certified only for the instrument we calibrated.
5. This result of calibration was found accurate as shown on date and place of calibration only.
6. Condition of Calibrated Item : Good

UIUC Description :

Time of Record 1 Hour 9 Minute At 41.5 °C

Fresh air Damper	-	Open	Position	-
	X	Close	Fan	1000
	-	Not Available		

- | | | | | |
|----------------------------|---|--------------------|--|------------------|
| 7. Result of Calibration : | X | Without adjustment | | After adjustment |
|----------------------------|---|--------------------|--|------------------|

S. Jørgensen
25 March 2021

F-CS-012 Revision: 01 Date: 20-04-65

Calibration Report

Certificate No.: 2502229-004-01
Equipment: CHAMBER (Incubator)
Model: IN75 Serial No.: D317.0305
Resolution: 0.1 °C ID No.: UAE.MIC.022/2561
Manufacturer: MEMMERT

Date of Calibration: 20 March 2025

Page 3 of 3

Calibration point: 41.5 °C

Calibration result:

Calibration Condition	Temperature (°C)	Relative Humidity (%)	Line Voltage (Volt)
MIN	28.6	58	220.0
MAX	28.9	60	225.0

Table 1 : Reporting of Temperature

Calibration point (°C)	Measured Temperature (°C) @ Sensor No. (Sensor No.9 is REF)									Uncertainty ± (°C)
	# 1	# 2	# 3	# 4	# 5	# 6	# 7	# 8	# 9	
41.5	41.50	41.39	41.45	41.40	41.69	41.35	41.29	41.32	41.34	0.27

Table 2 : Reporting of Characterization Result

UUC* Setting (°C)	UUC* Reading (°C)			Stability ± (°C)	Uniformity (°C)	Overall Variation (°C)
	MIN	MAX	Average			
41.5	41.5	41.5	41.5	0.023	0.34	0.44

Note: The quoted uncertainty include " Stability " and " Loading effect (20% of Temp Uniformity) "

UUC* = Unit Under Calibration

Stability = One-half of the greatest maximum difference of measured temperatures at any one sensors, for at least half an hour after reaching steady state.

Uniformity = The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time.

Overall Variation = The difference of the maximum and minimum measured temperatures throughout observation time.

The report uncertainty of measurement was based on standard uncertainty multiplied by coverage factor k= 2, providing a level of confidence of approximately 95 %.

----- End -----

F-CS-012 Revision: 01 Date: 20-04-65

2008 ถนนสุขุมวิท 36 แขวงคลองเตย เขตคลองเตย กรุงเทพมหานคร 10110
2008 So. 36 Anul Amn Road, Bang Yi Khan Subdistrict, Bang Phai District, Bangkok 10700, Thailand
Tel: +66(0) 2422 8888 Fax: +66(0) 2422 8545

เอกสารไม่ควบคุม
25 March 2025
nfi.com



Calibration Certificate

Certificate No.: 2502229-005-01
Client name: UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.
Address: 3 Soi Udomsuk 41, Sukhumvit Road, Bangchack, Prakhnong, Bangkok 10260

Page 1 of 3

Equipment: CHAMBER (Incubator)

Manufacturer: MEMMERT

Model: IN75

Serial No.: D317.0307

ID No.: UAE.MIC.023/2561

Order No.: 2502229

Operation No.: 2502229-005

Date of Receipt: 19 March 2025

Date of Calibration: 19 March 2025

Calibrated by Mr.Yothin Charoensuk Scientist

Approved by (Mr.Pheraphat Tuanjit) (for)

Manager, Division of Calibration Laboratory

Date of Issue: 25 March 2025

Responsible for the Technical Management Team

The uncertainties are for a confidence probability of approximately 95 %.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the National Food Institute.

F-CS-009 Revision: 01 Date: 20-04-65

2008 ถนนสุขุมวิท 36 แขวงคลองเตย เขตคลองเตย กรุงเทพมหานคร 10110
2008 So. 36 Anul Amn Road, Bang Yi Khan Subdistrict, Bang Phai District, Bangkok 10700, Thailand
Tel: +66(0) 2422 8888 Fax: +66(0) 2422 8545

เอกสารไม่ควบคุม
nfi.com



Calibration Report

Certificate No.: 2502229-005-01
Equipment: CHAMBER (Incubator)
Model: IN75 **Serial No.:** D317.0307
Resolution: 0.1 °C **ID No.:** UAE.MIC.023/2561
Manufacturer: MEMMERT
Date of Calibration: 19 March 2025

Page 2 of 3

Location: 302, UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.
Environment Condition: Ambient Temperature (20.9 ± 1) °C
Relative Humidity (59 ± 1) %
Line Voltage (223 ± 3) Volt

Condition of this results of Calibration:

- This instrument was calibrated by insert 9 standard thermometer into its chamber and calibration according to W-TE-014 Based on TLAS G-20-1/02-08 (E): Guidelines for Calibration and Checks of Temperature Controlled Enclosures.
- The temperature scale used was based on ITS - 90.
- All data show below were final values and the initial data may be obtained upon request.
- Reference Standard Instrument :

Instrument	Model	Serial No./ID No.	Certificate No.	Due Date	Through
Digital Thermometer with sensor	34972A	MY57003188	TE 670486-01	8 June 2025	NATIONAL FOOD INSTITUTE
	RTD	CH101-109/RTD A101-109			

- This certificate is traceable to International System of Units (SI Units).
- This certificate was certified only for the instrument we calibrated.
- This result of calibration was found accurate as shown on date and place of calibration only.
- Condition of Calibrated item : Good

UUC Description :

Time of Record 1 Hour 9 Minute At 41.0 °C
Fresh air Damper - Open Position -
X Close Fan -
- Not Available

- Result of Calibration : ☒ Without adjustment ☐ After adjustment

P. Janghalit
25 March 2025

F-CS-012 Revision: 01 Date: 20-04-65



Calibration Report

Certificate No.: 2502229-005-01
Equipment: CHAMBER (Incubator)
Model: IN75 **Serial No.:** D317.0307
Resolution: 0.1 °C **ID No.:** UAE.MIC.023/2561
Manufacturer: MEMMERT
Date of Calibration: 19 March 2025

Page 3 of 3

Calibration point: 41.0 °C

Calibration result:

Calibration Condition	Temperature (°C)	Relative Humidity (%)	Line Voltage (Volt)
MIN	20.6	58	220.0
MAX	21.2	60	225.0

Table 1 : Reporting of Temperature

Calibration point (°C)	Measured Temperature (°C) @ Sensor No. (Sensor No.9 is REF)									Uncertainty ± (°C)
	# 1	# 2	# 3	# 4	# 5	# 6	# 7	# 8	# 9	
41.0	41.78	41.48	41.56	41.50	41.11	41.05	40.87	41.00	41.06	0.34

Table 2 : Reporting of Characterization Result

UUC* Setting (°C)	UUC* Reading (°C)			Stability ± (°C)	Uniformity (°C)	Overall Variation (°C)
	MIN	MAX	Average			
41.0	41.0	41.0	41.0	0.12	0.72	1.1

Note: The quoted uncertainty include " Stability " and " Loading effect (20% of Temp Uniformity) "

UUC* = Unit Under Calibration

Stability = One-half of the greatest maximum difference of measured temperatures at any one sensors, for at least half an hour after reaching steady state.

Uniformity = The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time.

Overall Variation = The difference of the maximum and minimum measured temperatures throughout observation time.

The report uncertainty of measurement was based on standard uncertainty multiplied by coverage factor k= 2, providing a level of confidence of approximately 95 %.

----- End -----

P. Janghalit
25 March 2025

F-CS-012 Revision: 01 Date: 20-04-65





ศูนย์บริการห้องปฏิบัติการอุตสาหกรรมอาหาร
Foundation for Industrial Development National Food Institute
Food Industrial Laboratory Service Center




Calibration Certificate

Certificate No.: 2502229-001-01
Client name: UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.
Address: 3 Soi Udomsuk 41, Sukhumvit Road,
Bangchack, Prakhonong, Bangkok 10260

Page 1 of 3

Equipment: CHAMBER (Incubator)
Manufacturer: MEMMERT
Model: IPP 260
Serial No.: V615.0187
ID No.: UAE.MIC.003/2559
Order No.: 2502229
Operation No.: 2502229-001
Date of Receipt: 19 March 2025
Date of Calibration: 19 March 2025

Calibrated by Mr.Jerawut Prapawuttipong
Scientist

Approved by 
(Mr.Pheraphat Tuanjit) (for)
Manager, Division of Calibration Laboratory
Responsible for the Technical Management Team

Date of Issue: 25 March 2025

The uncertainties are for a confidence probability of approximately 95 %.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the National Food Institute.

F-CS-009 Revision: 01 Date: 20-04-65

2009 ๒๕๕๒ ถนนสุขุมวิท ๔๑ แขวงคลองเตย เขตคลองเตย กรุงเทพมหานคร 10๑๑๐๑ โทรศัพท์ ๐๒-๒๕๒๒ ๘๕๘๘ โทรสาร ๐๒-๒๕๒๒ ๘๕๔๕
2009 50-35 Anuram Road, Bang Y, Khan Subokand, Bang Phat Distric, Bangkok 10700, Thailand
Tel: +66(0) 2422 8588 Fax: +66(0) 2422 8545



ศูนย์บริการห้องปฏิบัติการอุตสาหกรรมอาหาร
Foundation for Industrial Development National Food Institute
Food Industrial Laboratory Service Center



Calibration Report

Certificate No.: 2502229-001-01
Equipment: CHAMBER (Incubator)
Model: IPP 260 **Serial No.:** V615.0187
Resolution: 0.1 °C **ID No.:** UAE.MIC.003/2559
Manufacturer: MEMMERT

Date of Calibration: 19 March 2025

Page 2 of 3

Location: LABORATORY, UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.
Environment Condition: Ambient Temperature (16.2 ± .3) °C
Relative Humidity (32 ± 4) %
Line Voltage (223 ± 3) Volt

Condition of this results of Calibration:

- This instrument was calibrated by insert 9 standard thermometer into its chamber and calibration according to W-TE-014 Based on TLAS G-20-1/02-08 (E): Guidelines for Calibration and Checks of Temperature Controlled Enclosures.
- The temperature scale used was based on ITS - 90.
- All data show below were final values and the initial data may be obtained upon request.
- Reference Standard Instrument :

Instrument	Model	Serial No./ID No.	Certificate No.	Due Date	Through
Digital Thermometer with sensor	34972A	MY49016851	TE 670477-01	4 May 2025	NATIONAL FOOD INSTITUTE
	RTD	CH101-109/ RTD#101-109			

- This certificate is traceable to International System of Units (SI Units).
- This certificate was certified only for the instrument we calibrated.
- This result of calibration was found accurate as shown on date and place of calibration only.
- Condition of Calibrated item : Good

UUC Description :

Time of Record i Hour 9 Minute At 35.0 °C
Fresh air Damper - Open Position -
X Close Fan -
- Not Available

- Result of Calibration : ☒ Without adjustment ☐ After adjustment


25 March 2025

F-CS-012 Revision: 01 Date: 20-04-65

2009 ๒๕๕๒ ถนนสุขุมวิท ๔๑ แขวงคลองเตย เขตคลองเตย กรุงเทพมหานคร 10๑๑๐๑ โทรศัพท์ ๐๒-๒๕๒๒ ๘๕๘๘ โทรสาร ๐๒-๒๕๒๒ ๘๕๔๕
2009 50-35 Anuram Road, Bang Y, Khan Subokand, Bang Phat Distric, Bangkok 10700, Thailand
Tel: +66(0) 2422 8588 Fax: +66(0) 2422 8545



Calibration Report

Certificate No.: 2502229-001-01
Equipment: CHAMBER (Incubator)
 Model: IPP 260 Serial No.: V615.0187
 Resolution: 0.1 °C ID No.: UAE.MIC.003/2559
 Manufacturer: MEMMERT

Date of Calibration: 19 March 2025

Page 3 of 3

Calibration point: 35.0 °C

Calibration result:

Calibration Condition	Temperature (°C)	Relative Humidity (%)	Line Voltage (Volt)
MIN	15.5	28	220.0
MAX	17.1	35	225.0

Table 1 : Reporting of Temperature

Calibration point (°C)	Measured Temperature (°C) @ Sensor No. (Sensor No.9 is REF)									Uncertainty ± (°C)
	# 1	# 2	# 3	# 4	# 5	# 6	# 7	# 8	# 9	
35.0	34.94	34.95	34.91	34.93	35.15	35.01	34.98	35.05	35.12	0.29

Table 2 : Reporting of Characterization Result

UUC* Setting (°C)	UUC* Reading (°C)			Stability ± (°C)	Uniformity (°C)	Overall Variation (°C)
	MIN	MAX	Average			
35.0	35.0	35.0	35.0	0.10	0.21	0.35

Note: The quoted uncertainty include * Stability * and * Loading effect (20% of Temp Uniformity) *

UUC* = Unit Under Calibration


Stability = One-half of the greatest maximum difference of measured temperatures at any one sensors, for at least half an hour after reaching steady state.

Uniformity = The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time.

Overall Variation = The difference of the maximum and minimum measured temperatures throughout observation time.

The report uncertainty of measurement was based on standard uncertainty multiplied by coverage factor k= 2, providing a level of confidence of approximately 95 %.

----- End -----


 25 March 2025

F-C5-012 Revision: 01 Date: 20-04-65

8008 ปตท. จำกัด (มหาชน) 8008 ปตท. จำกัด (มหาชน)
 8008 So. 36, Arun Amarin Road, Bang Yi Khan, Subdistrict, Bang Phli District, Bangkok 10700, Thailand
 Tel: +66(0) 2422 8688 Fax: +66(0) 2422 8545



Certificate of Calibration

Cert. No.: 25TM501
Page: 1 of 3

Equipment : Water Bath
Manufacturer : Memmert
Model : WNE 14
Serial No. : L414.1407
ID No. : UAE.MIC.006/2558
Submitted by : United Analyst and Engineering Consultant Co.,Ltd.
 3 Soi Udomsuk 41, Sukhumvit Road,
 Bangchak, Phrakhanong,
 Bangkok 10260
Location : Microbiology Laboratory (302)
Received Order : 19 March 2025
Calibration Date : 19 March 2025
Ambient Temperature : (26 ± 10) °C
Relative Humidity : (50 ± 30) %
AC Line Voltage : (220 ± 22) V

Calibrated by : Krisda Malee

Approved by :


 Approved Signatory

☐ Chakrit Waewwanjua
☐ Suwit Imjai
☒ Kunchit Promprat

Issue Date : 27 March 2025

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
 Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

เอกสารไม่ควบคุม



Equipment : Water Bath
 Condition As-Received : Used Item
 Reference : 2503-0436OC-1

Cert. No.: 25TM501
 Page : 2 of 3

Procedure Used :-

Calibration were conducted using in-house calibration procedure CP-OT04 Based on ASTM E715 according to direct measurement method with Data Acquisition which connected with Industrial Platinum Resistance Thermometer (IPRT).

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

Instrument	Serial No.	Cert. No.	Traceable	Due Date
1) Data Acquisition	MY57013823	23LM71	TPA	12 May 2025

2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certification is traceable to the International System of Unit.


Remark : TPA : Technology Promotion Association (Thailand - Japan)

Result of Calibration :- (*) Without Adjustment

Function of UUC* : Temperature Source

Heat transfer medium used : Water

	Environmental		AC Voltage Supply
	(°C)	(%R.H.)	(Volt)
Beginning of Calibration	24	50	220
Finished of Calibration	25	53	221

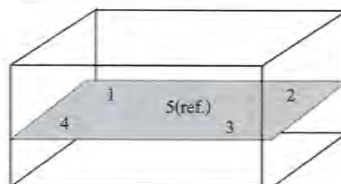

Front

Position :	Ref. Std. S/N.:
1	4804539-006
2	4804539-007
3	4804539-008
4	4804539-009
5(ref.)	4804539-010

เอกสารไม่ควบคุม



Equipment : Water Bath
 Condition As-Received : Used Item
 Reference : 2503-0436OC-1

Cert. No.: 25TM501
 Page : 3 of 3

Result of Calibration :- (*) Without Adjustment

Function of UUC* : Temperature Source

Calibration point (°C)	UUC* Setting (°C)	UUC* Reading (°C)	Average* Standard Reading (°C)					Uncertainty (± °C)
			Position					
			1	2	3	4	5 (ref.)	
44.5	44.4	44.4	44.508	44.531	44.495	44.537	44.510	0.15

Calibration point (°C)	Uniformity (°C)	Stability (± °C)	Coverage Factor k
44.5	0.092	0.048	2

Average* : The average of 30 values in each position.

Uniformity : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.

Stability : One-half of the greatest maximum difference of measured temperature at any one probe.

UUC* : Unit Under Calibration

Note : The reported uncertainty of measurement was included stability and excluded uniformity.

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

เอกสารไม่ควบคุม




TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL.0-2717-3000-29 FAX.0-2719-9484



Certificate of Calibration

Cert. No.: 25TM503
Page : 1 of 3

Equipment : Water Bath
Manufacturer : Memmert
Model : WNE 14
Serial No. : L414.1410
ID No. : UAE.MIC.015/2565
Submitted by : United Analyst and Engineering Consultant Co.,Ltd.
3 Soi Udomsuk 41, Sukhumvit Road,
Bangchak, Phrakhanong,
Bangkok 10260
Location : Microbiology Laboratory (302)
Received Order : 19 March 2025
Calibration Date : 19 March 2025
Ambient Temperature : (26 ± 10) °C
Relative Humidity : (50 ± 30.) %
AC Line Voltage : (220 ± 22) V
Calibrated by : Krisda Malee
Approved by : 
() Chakrit Waewwanjua
() Suwit Imjai
(✓) Kunchit Promprat
Issue Date : 27 March 2025

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3: Equipment Calibration and Testing Services.

เอกสารไม่ควบคุม



Equipment : Water Bath
Condition As-Received : Used Item
Reference : 2503-0436OC-3
Procedure Used :-

Cert. No.: 25TM503
Page : 2 of 3

Calibration were conducted using in-house calibration procedure CP-OT04 Based on ASTM E715 according to direct measurement method with Data Acquisition which connected with Industrial Platinum Resistance Thermometer (IPRT).

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

Instrument	Serial No.	Cert. No.	Traceable	Due Date
1) Data Acquisition	MY57013823	23LM71	TPA	12 May 2025

2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certification is traceable to the International System of Unit.


Remark : TPA : Technology Promotion Association (Thailand - Japan)

Result of Calibration :- (*) Without Adjustment

Function of UUC* : Temperature Source

Heat transfer medium used : Water

	Environmental		AC Voltage Supply
	(°C)	(%R.H.)	(Volt)
Beginning of Calibration	24	51	221
Finished of Calibration	25	52	220

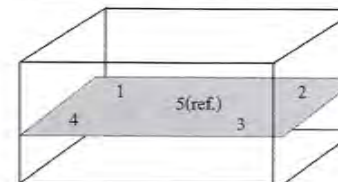

Front

Position :	Ref. Std. S/N.:
1	4804539-006
2	4804539-007
3	4804539-008
4	4804539-009
5(ref.)	4804539-010

เอกสารไม่ควบคุม



Equipment : Water Bath
 Condition As-Received : Used Item
 Reference : 2503-0436OC-3
 Result of Calibration :- (*) Without Adjustment
 Function of UUC* : Temperature Source

Cert. No.: 25TM503
 Page : 3 of 3

Calibration point (°C)	UUC* Setting (°C)	UUC* Reading (°C)	Average* Standard Reading (°C)					Uncertainty (± °C)
			Position					
			1	2	3	4	5 (ref.)	
44.5	44.5	44.5	44.533	44.509	44.527	44.518	44.517	0.15

Calibration point (°C)	Uniformity (°C)	Stability (± °C)	Coverage Factor <i>k</i>
44.5	0.057	0.038	2

Average* : The average of 30 values in each position.

Uniformity : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.

Stability : One-half of the greatest maximum difference of measured temperature at any one probe.

UUC* : Unit Under Calibration

Note : The reported uncertainty of measurement was included stability and excluded uniformity.

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-000-

เอกสารไม่ควบคุม



องค์การส่งเสริมและพัฒนาสถาบันอาหาร
 ศูนย์บริการห้องปฏิบัติการอาหาร
 Foundation for Industrial Development National Food Institute
 Food Industrial Laboratory Service Center



Calibration Certificate

Certificate No.: 2502227-001-01
 Client name: UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.
 Address: 3 Soi Udomsuk 41, Sukhumvit Road,
 Bangchack, Prakhong, Bangkok 10260

Page 1 of 3

Equipment: Electronic Balance

Manufacturer: OHAUS

Model: PX623

Serial No.: C236754745

ID No.: UAE.MIC.055/2565

Order No.: 2502227

Operation No.: 2502227-001

Date of Receipt: 19 March 2025

Date of Calibration: 19 March 2025

Calibrated by Mr.Yothin Charoensuk
 Scientist

Approved by *for N. mprubab*
 (Mr.Pheraphat Tuanjit)
 Manager, Division of Calibration Laboratory
 Responsible for the Technical Management Team

Date of Issue: 25 March 2025

The uncertainties are for a confidence probability of approximately 95%

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the National Food Institute.

FCS-009 Revision: 01 Date: 20-04-65

2008 ถนนสุขุมวิท 35 ถนนสุขุมวิท แขวงคลองตัน เขตคลองเตย กรุงเทพมหานคร 10700
 2008 Soi 35, Anah Ararat Road Bang Yi Khan Subdistrict, Bang Phra District, Bangkok 10700
 โทร : +66(0) 2122 8588 Fax : +66(0) 2122 8545



นฟิ.อิน

Calibration Report

Certificate No.: 2502227-001-01
Equipment: Electronic Balance
Model: PX623
Serial No.: C236754745
Capacity: 620
Manufacturer: OHAUS
Resolution: 0.001
ID No.: UAE.MJC.055/2565

Date of Calibration: 19 March 2025 Page 2 of 3

Environment Condition: Ambient Temperature: 22.8 ± 0.3 °C Relative Humidity: 51 ± 0.95 %

Place of Calibration: 301, UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.

Condition of Equipment: Good Condition

Condition of This Results of Calibration:

1. Calibration Method: NFI Method W-MA-001 In-House Method based on UKAS Lab 14 : 2019

2. Reference Standards:

Reference Standard	Model	Serial No.	Calibrated By	Certificate No.	Due Date
Standard Weight Class E2	1mg to 200g	B565567572	TCS	M24041005	19 April 2025
Standard Weight Class E2	500g	B565567696	TCS	M24041015	19 April 2025

Instrument	Model	Serial No.	Calibrated By	Certificate No.	Due Date
Thermo-Hygro Meter	608-H1	NFI.BTH.017/73	Quality Reborn	QR25-0542	10 February 2026

3. This certification is traceable to SI UNIT

4. This certificate was certified only for the instrument we calibrated.

5. This result of calibration was found accurate as shown on date and place of calibration only.

Calibration Results:

1. Repeatability of Reading:


Nominal Value (g)	Standard Deviation of Reading (g)
300	0.00042
600	0.00048

2. Off-Center Error:


A mass of 200 g was placed and moved to various position on pan.

The balance reading obtained is given in the table.


acing obtained is given in the table.



☐



☒



☐

1	2	3	4	5	6	(Maximum Difference)
(g)	(g)	(g)	(g)	(g)	(g)	(g)
200.002	200.003	200.001	200.001	200.002	200.002	0.001

FCS-012 Revision: 01 Date: 20-04-65

2008 ถนนสุขุมวิท 36 แขวงคลองเตย เขตวัฒนา กรุงเทพมหานคร 10170
2008 Soi 36, Arun Amarin Road, Bang Y. Khan Subdistrict, Bang Phli District, Bangkok 10170
Tel: +66(0) 2422 8589 Fax: +66(0) 2422 8545



nfi.or.th

Calibration Report

Certificate No.: 2502227-001-01
Equipment: Electronic Balance
Model: PX623
Serial No.: C236754745
Capacity: 620
Manufacturer: OHAUS
Resolution: 0.001
ID No.: UAE.MJC.055/2565

Date of Calibration: 19 March 2025 Page 3 of 3

Calibration Results: (Continued)

Calibration Range: 0-600 g

Calibration Adjustment: Internal Calibration

3. Departure from Nominal Value:

Nominal Value (g)	Standard Value (g)	Average Reading (g)	Correction (g)	Uncertainty (± g)	Coverage Factor k
Unload	0.0000	0.000	0.000	0.00086	2.00
1	1.0000	1.000	0.000	0.00086	2.00
5	5.0000	4.999	0.001	0.00086	2.00
10	10.0000	10.000	0.000	0.00086	2.00
20	20.0000	20.000	0.000	0.00086	2.00
50	50.0000	50.000	0.000	0.00087	2.00
100	100.0001	100.000	0.000	0.00087	2.00
200	200.0001	200.001	-0.001	0.00090	2.00
300	300.0002	300.001	-0.001	0.00094	2.00
400	400.0003	399.999	0.001	0.0011	2.00
500	500.0003	499.999	0.001	0.0011	2.00
600	600.0004	600.000	0.000	0.0012	2.00

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k , providing a level of confidence of approximately 95 %.

----- End -----

FCS-012 Revision: 01 Date: 20-04-65

2008 ถนนสุขุมวิท 36 แขวงคลองเตย เขตวัฒนา กรุงเทพมหานคร 10170
2008 Soi 36, Arun Amarin Road, Bang Y. Khan Subdistrict, Bang Phli District, Bangkok 10170
Tel: +66(0) 2422 8589 Fax: +66(0) 2422 8545



nfi.or.th

Calibration Certificate

Certificate No.: 2502229-007-01
Client name: UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.
Address: 3 Soi Udomsuk 41, Sukhumvit Road,
Bangchack, Prakhnong, Bangkok 10260

Page 1 of 3

Equipment: Autoclave
Manufacturer: ALP
Model: CL-40L
Serial No.: 808763
ID No.: UAE.MIC.026/2563
Order No.: 2502229
Operation No.: 2502229-007
Date of Receipt: 19 March 2025
Date of Calibration: 19 March 2025

Calibrated by Mr.Jerawut Prapawuttipong
Scientist

Approved by *P. Jenghahit*
(Mr.Pheraphat Tuanjit) (for)
Manager, Division of Calibration Laboratory
Responsible for the Technical Management Team

Date of Issue: 25 March 2025

The uncertainties are for a confidence probability of approximately 95 %.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the National Food Institute.

F-CS-009 Revision: 01 Date: 20-04-65

Calibration Report

Certificate No.: 2502229-007-01
Equipment: Autoclave
Model: CL-40L Serial No.: 808763
Resolution: 0.1 °C ID No.: UAE.MIC.026/2563
Manufacturer: ALP
Date of Calibration: 19 March 2025

Page 2 of 3

Location: LABORATORY, UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.
Environment Condition: Ambient Temperature (23 ± 1) °C
Relative Humidity (60 ± 5) %
Line Voltage (225 ± 1) Volt

Condition of this results of Calibration:

- This instrument was calibrated by insert 3 standard Data loggers with RTD into its autoclave and calibration according to W-TE-018 based on BS 2646-1:2021, Autoclaves for sterilization in laboratories
Part 1: Design, construction, safety and performance - Specification.
- The temperature scale used was based on ITS - 90.
- All data show below were final values and the initial data may be obtained upon request.

2. Reference Standard Instrument :

Instrument	Model	Serial No.	Certificate No.	Due Date	Through
Digital Thermometer with RTD (Data Logger)	HiTemp140-PT	S35646	TE 670370-01	23-Mar-25	NATIONAL FOOD INSTITUTE
	HiTemp140-PT	S33753	TE 670371-01	23-Mar-25	NATIONAL FOOD INSTITUTE
	HiTemp140-PT	S29973	TE 670372-01	23-Mar-25	NATIONAL FOOD INSTITUTE

- This certificate is traceable to International System of Units (SI Units).
- This certificate was certified only for the instrument we calibrated.
- This result of calibration was found accurate as shown on date and place of calibration only.
- This standard does not apply to sterilizers or disinfectors used for medical, dental, pharmaceutical.
- Condition of Calibrated item : Good

UUC Description : Setting program function sterilization : STERILIZE/NORMAL
Time of sterilization 15 Minute At 115.0 and 121.0°C

8. Result of Calibration : ☒ Without adjustment
☐ After adjustment

P. Jenghahit
25 March 2025

F-CS-012 Revision: 01 Date: 20-04-65

Calibration Report

Certificate No.: 2502229-007-01
Equipment: Autoclave
Model: CL-40L Serial No.: 808763
Resolution: 0.1 °C ID No.: UAE.MIC.026/2563
Manufacturer: ALP


Date of Calibration: 19 March 2025

Page 3 of 3

Calibration point: 115.0 and 121.0 °C

Calibration result:

Calibration Condition	Temperature (°C)	Relative Humidity (%)	Line Voltage (Volt)
Min	22.0	55	224
Max	24.0	65	226



Standard A-1 (Ref)
Sensor 1 is calibrated to the 115.0 °C temperature point.
Sensor 2 is the upper 1/3 of the chamber.
Sensor 3 is the bottom 1/3 of the chamber.

Table 1 : Reporting of Temperature

Calibration Point (°C)	Measured Temperature (°C) @ Sensor No. (Sensor No.2 is REF)			Uncertainty ± (°C)
	Std.# 1	Std.# 2 (Ref)	Std.# 3	
115.0	115.32	115.46	115.22	0.64
121.0	121.31	121.53	121.31	0.64

Table 2 : Reporting of Characterization Result

UUC* Setting (°C)	UUC* Reading				Stability ± (°C)	Uniformity (°C)	Overall Variation (°C)
	Min (°C)	Max (°C)	Average (°C)	MPa			
115.0	115.0	115.1	115.0	0.08	0.11	0.12	0.26
121.0	121.0	121.1	121.0	0.12	0.13	0.15	0.29

Note

The quoted uncertainty include " Stability " and " Loading effect (20% of Uniformity)"

UUC* = Unit Under Calibration

Stability = One-half of the greatest maximum difference of measured temperatures at any one sensors, for at least half an hour after reaching steady state.

Uniformity = The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time.

Overall Variation = The difference of the maximum and minimum measured temperatures throughout observation time.

The report uncertainty of measurement was based on standard uncertainty multiplied by coverage factor k= 2, providing a level of confidence of approximately 95 %.

----- End -----

P. Janyabait
25 March 2025

F-CS-012 Revision: 01 Date: 20-04-65



Certificate of Calibration

Certificate No. : 68-420062-1

Page : 1 of 2

Submitted by : Pacific Laboratory Co., Ltd.

14/5358 Moo 14, T. Bang Bua Thong, A. Bang Bua Thong, Nonthaburi 11110 Thailand

Equipment : pH Meter with electrode

pH meter

Manufacturer : Eutech

Model : pH 700

Range : N/A pH

Resolution : 0.01 pH

Serial No. : 2841305

ID No. : LAB-PH-002

Electrode

Model : N/A

Serial No. : 3172493

Environment : On site calibration was carried out at the Laboratory, Pacific Laboratory Co., Ltd.

Ambient Temperature : (23.5 to 25.0)° C

Relative Humidity : (50 to 55) %

Date of Received : 21 July 2025

Date of Calibration : 21 July 2025

Date of Issue : 24 July 2025

Calibrated by : Permpon Chanpu

Calibration Method : In-house method CAL-M4201 direct measurement by using standard voltage calibrator and using certified reference material (CRM)

Reference Standard Instruments : This certification is traceable to the International System of Units

1. Multiproduct Calibrator

ID No.	Cert. No.	Due Date	Traceability
400005	SG-E-00307/66	23 Aug 2025	National Institute of Metrology Thailand (NIMT)

2. Standard Buffer Solution

pH	Cert. No.	Lot No.	Exp. Date	Traceability
4.007	61314276	1081108	28 Feb 2027	CPA Chem Ltd. Accredited to ISO 17034 and ISO/IEC 17025
6.965	61318175	1081110	28 Feb 2026	CPA Chem Ltd. Accredited to ISO 17034 and ISO/IEC 17025
10.010	61325043	1081109	28 Feb 2026	CPA Chem Ltd. Accredited to ISO 17034 and ISO/IEC 17025

Approved by :



(Permpon Chanpu)

Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 68-420062-1

Page : 2 of 2

Result of Calibration :

UUC Condition As-Received : Good

Function : Electrical measurement

pH meter

Performing standard curve by Multiproduct Calibrator at pH (4,7,10)

Adjustment Curve at nominal pH	Applied Voltage (mV)	Nominal Value (pH)	UUC Reading		Correction (mV)	Uncertainty (± mV)
			(pH)	(mV)		
4, 7, 10	177.4800	4	4.00	177.5	0.0	0.12
	0.0000	7	7.00	0.1	-0.1	0.086
	-177.4800	10	10.00	-177.4	-0.1	0.12

Function : pH meter with electrode

Performing a three - buffer standard curve using buffer nominal pH (4,7,10)

Adjustment Curve at nominal pH	Standard Buffer (pH)	UUC Reading (pH)	Correction (pH)	Uncertainty (± pH)
4, 7, 10	4.007	4.01	0.00	0.0097
	6.965	7.00	-0.03	0.011
	10.010	10.01	0.00	0.014

Remark

UUC : Unit Under Calibration

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurment was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

- 000 -



Certificate of Calibration

Certificate No. : 68-420062-2

Page : 1 of 2

Submitted by : Pacific Laboratory Co., Ltd.

14/5358 Moo 14, T. Bang Bua Thong, A. Bang Bua Thong, Nonthaburi 11110 Thailand

Equipment : pH Meter with electrode

pH meter

Manufacturer : Eutech

Model : pH 700

Range : N/A pH

Resolution : 0.01 pH

Serial No. : 2841305

ID No. : LAB-PH-002

Electrode

Model : N/A

Serial No. : 3052953

Environment : On site calibration was carried out at the Laboratory, Pacific Laboratory Co., Ltd.

Ambient Temperature : (23.5 to 25.0)° C

Relative Humidity : (50 to 55) %

Date of Received : 21 July 2025

Date of Calibration : 21 July 2025

Date of Issue : 24 July 2025

Calibrated by : Permpon Chanpu

Calibration Method : In-house method CAL-M4201 direct measurement by using standard voltage calibrator and using certified reference material (CRM)

Reference Standard Instruments : This certification is traceable to the International System of Units

1. Multiproduct Calibrator

ID No.	Cert. No.	Due Date	Traceability
400005	SG-E-00307/66	23 Aug 2025	National Institute of Metrology Thailand (NIMT)

2. Standard Buffer Solution

pH	Cert. No.	Lot No.	Exp. Date	Traceability
4.007	61314276	1081108	28 Feb 2027	CPA Chem Ltd. Accredited to ISO 17034 and ISO/IEC 17025
6.965	61318175	1081110	28 Feb 2026	CPA Chem Ltd. Accredited to ISO 17034 and ISO/IEC 17025
10.010	61325043	1081109	28 Feb 2026	CPA Chem Ltd. Accredited to ISO 17034 and ISO/IEC 17025

Approved by :



(Permpon Chanpu)

Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 68-420062-2

Page : 2 of 2

Result of Calibration :

UUC Condition As-Received : Good

Function : Electrical measurement

pH meter

Performing standard curve by Multiproduct Calibrator at pH (4,7,10)

Adjustment Curve at nominal pH	Applied Voltage (mV)	Nominal Value (pH)	UUC Reading		Correction (mV)	Uncertainty (± mV)
			(pH)	(mV)		
4, 7, 10	177.4800	4	4.00	177.5	0.0	0.12
	0.0000	7	7.00	0.1	-0.1	0.086
	-177.4800	10	10.00	-177.4	-0.1	0.12

Function : pH meter with electrode

Performing a three - buffer standard curve using buffer nominal pH (4,7,10)

Adjustment Curve at nominal pH	Standard Buffer (pH)	UUC Reading (pH)	Correction (pH)	Uncertainty (± pH)
4, 7, 10	4.007	4.01	0.00	0.0097
	6.965	7.00	-0.03	0.011
	10.010	10.01	0.00	0.014

Remark

UUC : Unit Under Calibration

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurment was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

- 000 -



Certificate of Calibration

Certificate No. : 68-400421-1

Page : 1 of 2

Submitted by : Pacific Laboratory Co., Ltd.

14/5358 Moo 14, T. Bang Bua Thong, A. Bang Bua Thong, Nonthaburi 11110 Thailand

Equipment : Temperature Indicator with Thermistor Probe

Temperature Indicator

Manufacturer : Eutech

Model : pH 700

Range : N/A °C

Resolution : 0.1 °C

Serial No. : 2841305

ID No. : LAB-PH-002

Thermistor probe

Model : N/A

Sheath Material : Stainless

Diameter : 3 mm.

Length : 115 mm.

Serial No. : PHSTEMB01P 049

ID No. : LAB-PH-002

Environment : On site calibration was carried out at the Laboratory, Pacific Laboratory Co., Ltd.

Ambient Temperature : (23.5 to 25.0) °C

Relative Humidity : (50 to 55) %

Line Voltage : (220.0 to 221.0) VAC

Date of Received : 21 July 2025

Date of Calibration : 21 July 2025

Date of Issue : 24 July 2025

Calibrated by : Permpon Chanpu

Calibration Method : This instrument was calibrated by In-house method comparison technique CAL-M4003 by compared with PRT in the liquid bath at the constant controlled temperature.

The temperature scale used was based on ITS-90

Reference Standard Instruments : This certification is traceable to the International System of Units

1. Platinum Resistance Thermometer (PRT)

ID No.	Cert. No.	Due Date
400016	TT-1019-25	13 May 2027

Traceability

National Institute of Metrology Thailand (NIMT)

2. Standard Digital Thermometer

ID No.	Cert. No.	Due Date
400033	24E633	21 Feb 2026

Traceability

National Institute of Metrology Thailand (NIMT)

Approved by :



(Permpon Chanpu)

Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhprachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech.cal@yahoo.com, calibratech.cal@hotmail.com

Certificate of Calibration

Certificate No. : 68-400421-1

Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Function : Temperature measurement

Immersion Depth (mm.)	Standard Reading (°C)	UUC Reading (°C)	Correction (°C)	Uncertainty (± °C)
115	25.002	24.9	0.1	0.19

Remark

UUC : Unit Under Calibration

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

- ๐0๐ -



CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhaphrachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech.cal@yahoo.com, calibratech.cal@hotmail.com



NSC-TISI-TIS 17025
CALIBRATION 0030

Certificate of Calibration

Certificate No. : 68-400420-3

Page : 1 of 2

Submitted by : Pacific Laboratory Co., Ltd.

14/5358 Moo 14, T. Bang Bua Thong, A. Bang Bua Thong, Nonthaburi 11110 Thailand

Equipment : Temperature controlled enclosure (Incubator)

Manufacturer : Aqua Lytic

Model : TC 135S

Range : N/A °C

Resolution : 0.1 °C

Serial No. : 0614/000033

ID No. : LAB-IB-001

Environment : On site calibration was carried out at the Laboratory, Pacific Laboratory Co., Ltd.

Ambient Temperature : (23.0 to 24.5) °C

Relative Humidity : (40 to 45) %

Line Voltage : (220.0 to 222.0) V

Date of Received : 21 July 2025

Date of Calibration : 21 July 2025

Date of Issue : 24 July 2025

Calibrated by : Permpon Chanpu

Calibration Method : CAL-M4004, TLAS G-20

The temperature scale used was based on ITS-90

Reference Standard Instruments : This certification is traceable to the International System of Units
Standard Digital Thermometer with RTD Probe

ID No.

Cert. No.

Due Date

Traceability

400029 & 400048

68-400063-1

01 Aug 2025

National Institute of Metrology Thailand (NIMT)

Approved by :

(Permpon Chanpu)

Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 68-400420-3


Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Function : Temperature measurement

This instrument was setting air ventilation at position 0 (close)

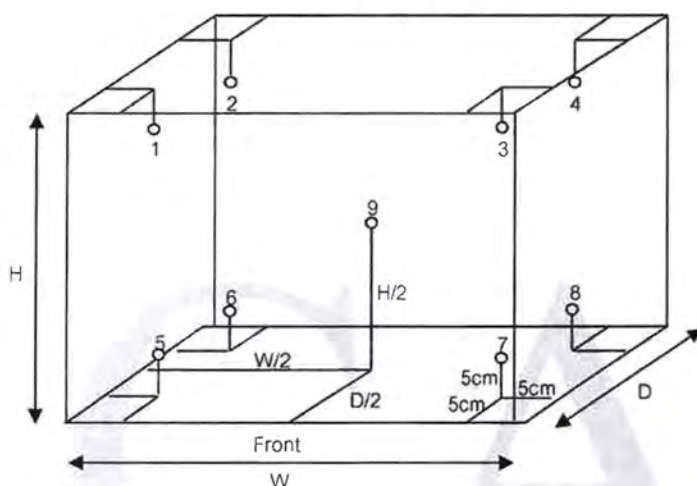

Inside of Chamber

W = 0.51 m

D = 0.04 m

H = 0.70 m

Capacity = 0.02 m³

Test Point (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Temperature (°C) @ Sensor No.									Uncertainty (± °C)
			1	2	3	4	5	6	7	8	9	
20.0	20.5	20.5	20.10	19.94	19.99	19.96	19.92	19.90	20.02	19.99	19.87	0.69

Test Point (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Uniformity (°C)	Measured Stability (°C)	Overall Variation (°C)
20.0	20.5	20.5	0.43	0.36	0.78

Remark The uncertainty is not combine uniformity of the air chamber

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

- o0o -

[Signature]



CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhprachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech.cal@yahoo.com, calibratech.cal@hotmail.com



NSC-TISI-TIS17025
CALIBRATION 0030

Certificate of Calibration

Certificate No. : 68-400420-2

Page : 1 of 2

Submitted by : Pacific Laboratory Co., Ltd.

14/5358 Moo 14, T. Bang Bua Thong, A. Bang Bua Thong, Nonthaburi 11110 Thailand

Equipment : Water Bath

Manufacturer : Memmert

Model : WNB 22

Range : N/A °C

Resolution : 0.1 °C

Serial No. : L514.0184

ID No. : LAB-WB-001

Environment : On site calibration was carried out at the Laboratory, Pacific Laboratory Co., Ltd.

Ambient Temperature : (31.0 to 31.8) °C

Relative Humidity : (50 to 55) %

Line Voltage : (220.0 to 222.0) V

Date of Received : 21 July 2025

Date of Calibration : 21 July 2025

Date of Issue : 24 July 2025

Calibrated by : Permpon Chanpu

Calibration Method : This instrument was calibrated by In-house method CAL-M4006 based on ASTM E715-80
The temperature scale used was based on ITS-90

Reference Standard Instruments : This certification is traceable to the International System of Units
Standard Digital Thermometer with RTD probe

<u>ID No.</u>	<u>Cert. No.</u>	<u>Due Date</u>	<u>Traceability</u>
400029 & 400031	68-400214-1	25 Oct 2025	National Institute of Metrology Thailand (NIMT)

Approved by :

(Permpon Chanpu)

Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration


Certificate No. : 68-400420-2

Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Function : Temperature measurement

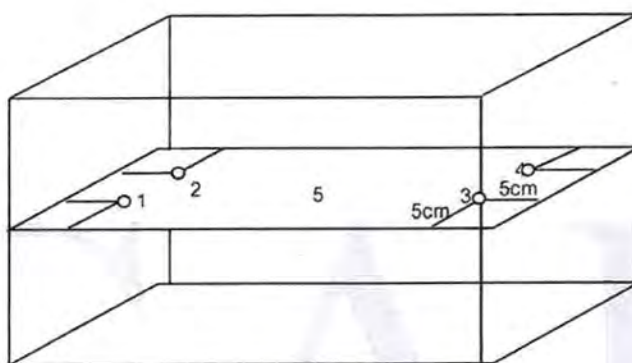

Front

Test Point (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Temperature (°C) @					Uncertainty (± °C)	Measured Uniformity (°C)	Measured Stability (°C)
			Sensor No.							
			1	2	3	4	5			
65.0	65.0	65.0	64.62	64.64	64.64	64.63	64.63	0.18	0.05	0.03
95.0	95.0	95.0	94.60	94.61	94.63	94.68	94.58	0.18	0.17	0.05

Remark The uncertainty is not combine uniformity of the water bath

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

- o0o -



CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhaphrasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech.cal@yahoo.com, calibratech.cal@hotmail.com



NSC-TISI-TIS 17025
CALIBRATION 0030

Certificate of Calibration

Certificate No. : 68-400420-1

Page : 1 of 2

Submitted by : Pacific Laboratory Co., Ltd.

14/5358 Moo 14, T. Bang Bua Thong, A. Bang Bua Thong, Nonthaburi 11110 Thailand

Equipment : Temperature controlled enclosure (Oven)

Manufacturer : Memmert

Model : UN 55

Range : N/A °C

Resolution : 0.1 °C

Serial No. : B214.1879

ID No. : LAB-OV-001

Environment : On site calibration was carried out at the Laboratory, Pacific Laboratory Co., Ltd.

Ambient Temperature : (31.0 to 31.8) °C

Relative Humidity : (50 to 55) %

Line Voltage : (220.0 to 222.0) V

Date of Received : 21 July 2025

Date of Calibration : 21 July 2025

Date of Issue : 24 July 2025

Calibrated by : Permpon Chanpu

Calibration Method : CAL-M4004, TLAS G-20

The temperature scale used was based on ITS-90

Reference Standard Instruments : This certification is traceable to the International System of Units
Standard Digital Thermometer with Thermocouple probe

<u>ID No.</u>	<u>Cert. No.</u>	<u>Due Date</u>	<u>Traceability</u>
400029 & 400032	68-400217-1	28 Oct 2025	National Institute of Metrology Thailand (NIMT)

Approved by :

(Permpon Chanpu)

Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.





Foundation for Industrial Development National Food Institute
Food Industrial Laboratory Service Center

NSC-TISI-TIS 170
CALIBRATION CO

Calibration Certificate

Certificate No.: 2502229-006-01
Client name: UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.
Address: 3 Soi Udomsuk 41, Sukhumvit Road,
 Bangchack, Prakhnong, Bangkok 10260

Page 1 of 3

Equipment: CHAMBER (Incubator)

Manufacturer: **BINDER**

Model: KB 400

Serial No.: 20200000015535

ID No.: UAE.MTC.018/2564

Order No.: 2502229

Operation No.: 2502229-006

Date of Receipt: 19 March 2025

Date of Calibration: 19 March 2025

Calibrated by Mr.Jerawut Prapawuttipong
Scientist

Approved by *J. Jangthakul*
(Mr. Pheraphat Tuanjit) (for)
Manager, Division of Calibration Laboratory
Responsible for the Technical Management Team

Date of Issue: 25 March 2025

The uncertainties are for a confidence probability of approximately 95 %.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the National Food Institute.

F-CS-009 Revision: 01 Date: 20-04-65

เอกสารไม่ควบคุม



infected

2008 Bangkok, 36 Pwasaung Road, Bang Y Kham Subdistrict, Bang Phat District, Bangkok 10700, Thailand
Tel: +66(0) 2422 8888 Fax: +66(0) 2422 8545

၂၀၁၆ ခုနှစ် ဖွဲ့စည်းပုံအခြေခံဥပဒေ

List Certificate of Laboratory Instrument

No.	Instrument/Equipment	Parameter	Manufacturer	Model/Serial No.	Calibrator	Certification No.	Date of Calibration	Due date of Calibration*	Remark
Laboratory Instrument for Water Quality Analysis									
1	Incubator	Torik Coliform System (5 Cell)	Mettler	KB0000 / J5000000015336	National Food Institute, Ministry of Industry, Thailand	2502229 028 01	19 Mar 25	18 Mar 26	-
2	Incubator	Conductivity Pen/Pengisi Japonica app		W 19.3 / 511 02391	National Food Institute, Ministry of Industry, Thailand	2502229 028 01	30 Mar 25	19 Mar 26	-
3	Incubator	Staphylococcus Aureus, Pseudomonas, Aeromonas		BT 15.4 / 001 06833	National Food Institute, Ministry of Industry, Thailand	2502229 028 01	20 Mar 25	19 Mar 26	-
4	Incubator			BP 240.1 / 001510301	National Food Institute, Ministry of Industry, Thailand	2502229 028 01	19 Mar 25	18 Mar 26	-
5	Water Bath		Mettler	WBB 18.1 / 121610057	Technology Promotion Association (Thailand) (agri)	25176501	19 Mar 25	18 Mar 26	-
6	Water Bath			WBB 18.1 / 141613412	Technology Promotion Association (Thailand) (agri)	25176501	19 Mar 25	18 Mar 26	-
7	Analysis Balance		OHAUS	PK325 / C236254165	National Food Institute, Ministry of Industry, Thailand	2502229 0401 401	19 Mar 25	18 Mar 26	-
8	Auto-Clave			CL400 / 004243	National Food Institute, Ministry of Industry, Thailand	2502229 027 01	19 Mar 25	18 Mar 26	-

Due Date of Calibration: Based on the annual calibration plan. At least 1 time per year.

© 2006 Pearson Education, Inc. All rights reserved. Printed in the United States of America.

เอกสารไม่ควบคุม

1000-0000/01/0000-0000\$05.00/0

008 So-38, Anun Acharn Road, Bang Y Khan Subdistrict, Bang Phat District, Bangkok 10700, Thailand
+66(0) 2-232 6995 Fax +66(0) 2-422 8545

Calibration Report

Certificate No.: 2502229-006-01
Equipment: CHAMBER (Incubator)
Model: KB 400 Serial No.: 20200000015535
Resolution: 0.1 °C ID No.: UAE.MIC.018/2564
Manufacturer: BINDER
Date of Calibration: 19 March 2025

Page 2 of 3

Location: LABORATORY, UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.
Environment Condition: Ambient Temperature (18 ± 1) °C
Relative Humidity (50 ± 5) %
Line Voltage (223 ± 3) Volt

Condition of this results of Calibration:

- This instrument was calibrated by insert 13 standard thermometer into its chamber and calibration according to W-TE-014 Based on TLAS G-20-1/02-08 (E): Guidelines for Calibration and Checks of Temperature Controlled Enclosures.
- The temperature scale used was based on ITS - 90.
- All data show below were final values and the initial data may be obtained upon request.

2. Reference Standard Instrument :

Instrument	Model	Serial No./ID No.	Certificate No.	Due Date	Through
Digital Thermometer with sensor	34972A RTD	MY49016851 CH#201-303 / RTD#201-303	TE 670477-01	4 May 2025	NATIONAL FOOD INSTITUTE

- This certificate is traceable to International System of Units (SI Units).
- This certificate was certified only for the instrument we calibrated.
- This result of calibration was found accurate as shown on date and place of calibration only.
- Condition of Calibrated item : Good

UUC Description :

Time of Record 1 Hour 9 Minute At 35.0 °C
Fresh air Damper - Open Position -
X Close Fan -
- Not Available

7. Result of Calibration : ☒ Without adjustment: ☐ After adjustment

P. Jongsakulkit
25 March 2025

F-CS-012 Revision: 01 Date: 20-04-65



Calibration Report

Certificate No.: 2502229-006-01
Equipment: CHAMBER (Incubator)
Model: KB 400 Serial No.: 20200000015535
Resolution: 0.1 °C ID No.: UAE.MIC.018/2564
Manufacturer: BINDER
Date of Calibration: 19 March 2025

Page 3 of 3

Calibration point: 35.0 °C

Calibration result:

Calibration Condition	Temperature (°C)	Relative Humidity (%)	Line Voltage (Volt)
MIN	17.3	45	220.0
MAX	18.1	55	225.0

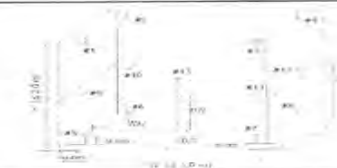


Table1 : Reporting of Temperature

Calibration point (°C)	Measured Temperature (°C) @ Sensor No. (Sensor No.13 is REF)													Uncertainty ± (°C)
	# 1	# 2	# 3	# 4	# 5	# 6	# 7	# 8	# 9	# 10	# 11	# 12	# 13	
35.0	34.98	35.17	34.99	34.92	35.18	35.01	35.00	35.13	35.00	34.96	35.02	35.17	35.04	0.27

Table 2 : Reporting of Characterization Result

UUC* Setting (°C)	UUC* Reading (°C)			Temperature Stability ± (°C)	Temperature Uniformity (°C)	Overall Variation (°C)
	MIN	MAX	Average			
35.0	35.0	35.0	35.0	0.029	0.15	0.30

Note: The quoted uncertainty include " Stability " and " Loading effect (20% of Temp Uniformity) "

UUC* = Unit Under Calibration

Stability = One-half of the greatest maximum difference of measured temperatures at any one sensors, for at least half an hour after reaching steady state.

Uniformity = The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time.

Overall Variation = The difference of the maximum and minimum measured temperatures throughout observation time.

The report uncertainty of measurement was based on standard uncertainty multiplied by coverage factor k=2, providing a level of confidence of approximately 95 %.

----- End -----

P. Jongsakulkit
25 March 2025

F-CS-012 Revision: 01 Date: 20-04-65



Calibration Certificate

Certificate No.: 2502229-004-01
Client name: UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.
Address: 3 Soi Udomsuk 41, Sukhumvit Road,
Bangchack, Prakhnong, Bangkok 10260

Page 1 of 3

Equipment: CHAMBER (Incubator)
Manufacturer: MEMMERT
Model: IN75
Serial No.: D317.0305
ID No.: UAE.MIC.022/2561
Order No.: 2502229
Operation No.: 2502229-004
Date of Receipt: 19 March 2025
Date of Calibration: 20 March 2025

Calibrated by Mr.Yothin Charoensuk
Scientist

Approved by *P. Jenghabut*
(Mr.Pheraphat Tuanjit) (for)
Manager, Division of Calibration Laboratory
Responsible for the Technical Management Team

Date of Issue: 25 March 2025

The uncertainties are for a confidence probability of approximately 95 %.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the National Food Institute.

F-CS-009 Revision: 01 Date: 20-04-65



Calibration Report

Certificate No.: 2502229-004-01
Equipment: CHAMBER (Incubator)
Model: IN75 **Serial No.:** D317.0305
Resolution: 0.1 °C **ID No.:** UAE.MIC.022/2561
Manufacturer: MEMMERT
Date of Calibration: 20 March 2025

Page 2 of 3

Location: 302, UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.
Environment Condition: Ambient Temperature (26.8 ± 1) °C
Relative Humidity (59 ± 1) %
Line Voltage (223 ± 3) Volt

Condition of this results of Calibration:

- This instrument was calibrated by insert 9 standard thermometer into its chamber and calibration according to W-TE-014 Based on TLAS G-20-1/02-08 (E): Guidelines for Calibration and Checks of Temperature Controlled Enclosures.
- The temperature scale used was based on ITS - 90.
- All data show below were final values and the initial data may be obtained upon request.
- Reference Standard Instrument :

Instrument	Model	Serial No./ID No.	Certificate No.	Due Date	Through
Digital Thermometer with sensor	34972A	MYS7003188	TE 670486-01	8 June 2025	NATIONAL FOOD INSTITUTE
	RTD	CH#101-109/ RTD#101-109			

- This certificate is traceable to International System of Units (SI Units).
- This certificate was certified only for the instrument we calibrated.
- This result of calibration was found accurate as shown on date and place of calibration only.
- Condition of Calibrated item : Good

UUC Description :

Time of Record : 1 Hour 9 Minute At 41.5 °C
Fresh air Damper : - Open Position -
Close Fan 100%
Not Available

- Result of Calibration : ☒ Without adjustment ☐ After adjustment.

F-CS-012 Revision: 01 Date: 20-04-65





ศูนย์บริการห้องปฏิบัติการอุตสาหกรรมอาหาร
Foundation for Industrial Development National Food Institute
Food Industrial Laboratory Service Center



Calibration Report

Certificate No.: 2502229-001-01
Equipment: CHAMBER (Incubator)
Model: IN75 Serial No.: D317.0305
Resolution: 0.1 °C ID No.: UAE.MIC.022/2561
Manufacturer: MEMMERT

Date of Calibration: 20 March 2025

Page 3 of 3

Calibration point: 41.5 °C

Calibration result:

Calibration Condition	Temperature (°C)	Relative Humidity (%)	Line Voltage (Volt)
MIN	28.6	58	220.0
MAX	28.9	60	225.0

Table1 : Reporting of Temperature

Calibration point (°C)	Measured Temperature (°C) @ Sensor No. (Sensor No.9 is REF)									Uncertainty ± (°C)
	# 1	# 2	# 3	# 4	# 5	# 6	# 7	# 8	# 9	
41.5	41.50	41.39	41.45	41.40	41.69	41.35	41.29	41.32	41.34	0.27

Table 2 : Reporting of Characterization Result

UUC* Setting (°C)	UUC* Reading (°C)			Stability ± (°C)	Uniformity (°C)	Overall Variation (°C)
	MIN	MAX	Average			
41.5	41.5	41.5	41.5	0.023	0.34	0.44

Note: The quoted uncertainty include " Stability " and " Loading effect (20% of Temp Uniformity) ".

UUC* = Unit Under Calibration

Stability = One-half of the greatest maximum difference of measured temperatures at any one sensors, for at least half an hour after reaching steady state.

Uniformity = The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time.

Overall Variation = The difference of the maximum and minimum measured temperatures throughout observation time.

The report uncertainty of measurement was based on standard uncertainty multiplied by coverage factor k= 2, providing a level of confidence of approximately 95 %.

----- End -----

F-CS-012 Revision: 01 Date: 20-04-65

2008 ถนนสุขุมวิท 35 แขวงคลองเตย เขตคลองเตย กรุงเทพมหานคร 10110
2008 Soi 35, Anin Anan Road, Bang Yai Khan Suddasit, Bangkok 10110, Thailand
Tel: +66(0) 2262 8508 Fax: +66(0) 2262 8545

เอกสารไม่ควบคุม



ศูนย์บริการห้องปฏิบัติการอุตสาหกรรมอาหาร
Foundation for Industrial Development National Food Institute
Food Industrial Laboratory Service Center



Calibration Certificate

Certificate No.: 2502229-005-01
Client name: UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.
Address: 3 Soi Udomsuk 41, Sukhumvit Road,
Bangchack, Prakhonong, Bangkok 10260

Page 1 of 3

Equipment: CHAMBER (Incubator)

Manufacturer: MEMMERT

Model: IN75

Serial No.: D317.0307

ID No.: UAE.MIC.023/2561

Order No.: 2502229

Operation No.: 2502229-005

Date of Receipt: 19 March 2025

Date of Calibration: 19 March 2025

Calibrated by Mr.Yothin Charoensuk
Scientist

Approved by *P. Pheraphat*
(Mr.Pheraphat Tuanjit) (for)

Manager, Division of Calibration Laboratory
Responsible for the Technical Management Team

Date of Issue: 25 March 2025

The uncertainties are for a confidence probability of approximately 95 %.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the National Food Institute.

F-CS-009 Revision: 01 Date: 20-04-65

2008 ถนนสุขุมวิท 35 แขวงคลองเตย เขตคลองเตย กรุงเทพมหานคร 10110
2008 Soi 35, Anin Anan Road, Bang Yai Khan Suddasit, Bangkok 10110, Thailand
Tel: +66(0) 2262 8508 Fax: +66(0) 2262 8545

เอกสารไม่ควบคุม



Calibration Report

Certificate No.: 2502229-005-01
Equipment: CHAMBER (Incubator)
Model: IN75 Serial No.: D317.0307
Resolution: 0.1 °C ID No.: UAE.MIC.023/2561
Manufacturer: MEMMERT

Date of Calibration: 19 March 2025

Page 2 of 3

Location: 302, UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.

Environment Condition:

Ambient Temperature	(20.9 ± 1) °C
Relative Humidity	(59 ± 1) %
Line Voltage	(223 ± 3) Volt.

Condition of this results of Calibration:

1. This instrument was calibrated by insert 9 standard thermometer into its chamber and calibration according to WTE-014 Based on TLAS G-20-1/02-08 (E): Guidelines for Calibration and Checks of Temperature Controlled Enclosures.
- The temperature scale used was based on ITS - 90.
 - All data show below were final values and the initial data may be obtained upon request.

Instrument	Model	Serial No./ID No.	Certificate No.	Due Date	Through
Digital Thermometer with sensor	34972A	MY57003188	TE 670486-01	8 June 2025	NATIONAL FOOD INSTITUTE
	RTD	CH#101-109/ RTD#101-109			

3. This certificate is traceable to International System of Units (SI Units).
4. This certificate was certified only for the instrument we calibrated.
5. This result of calibration was found accurate as shown on date and place of calibration only.
6. Condition of Calibrated item : Good

UUC Description

Time of Record 1 Hour 9 Minute At 41.0 °C

Fresh air Damper	-	Open	Position	-
	X	Close	Fan	-
	-	Not Available		

7. Result of Calibration : ☐ X Without adjustment ☐ After adjustment

F-CS-012 Revision: 01 Date: 20-04-65

2018-69 35, Anin Aneem Road, Bang Y Krai Subdistrict, Bang Phai District, Bangkok 10700, Thailand
Tel: +66(0) 2122 6868, Fax: +66(0) 2122 8545



of 0.57

Calibration Report

Certificate No.: 2502229-005-01
Equipment: CHAMBER (Incubator)
Model: IN75 Serial No.: D317.0307
Resolution: 0.1 °C ID No.: UAE.MIC.023/2561
Manufacturer: MEMMERT

Date of Calibration: 19 March 2025

Page 3 of 3

Calibration point: 41.0 °C

Calibration result:

Calibration Condition	Temperature (°C)	Relative Humidity (%)	Line Voltage (Volt)
MIN	20.6	58	220.0
MAX	21.2	60	225.0




Table1 : Reporting of Temperature

Calibration point (°C)	Measured Temperature (°C) @ Sensor No. (Sensor No.9 is REF)									Uncertainty ± (°C)
	# 1	# 2	# 3	# 4	# 5	# 6	# 7	# 8	# 9	
41.0	41.78	41.48	41.56	41.50	41.11	41.05	40.87	41.00	41.06	0.34

Table 2 : Reporting of Characterization Result

UUC* Setting (°C)	UUC* Reading (°C)			Stability ± (°C)	Uniformity (°C)	Overall Variations (°C)
	MIN	MAX	Average			
41.0	41.0	41.0	41.0	0.12	0.72	1.1

Note: The quoted uncertainty include "Stability" and "Loading effect (20% of Temp Uniformity)".

UUC* = Unit Under Calibration

Stability = One-half of the greatest maximum difference of measured temperatures at any one sensors, for at least half an hour after reaching steady state.

Uniformity = The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time.

Overall Variation = The difference of the maximum and minimum measured temperatures throughout observation time

The report uncertainty of measurement was based on standard uncertainty multiplied by coverage factor $k = 2$, providing a level of confidence of approximately 95 %.

----- End -----

FCS-012 Revision: 01 Date: 20-04-65

2008 ๒๕๕๑/๒๕๕๒-๓๐ นวตาสถาปนา สันติสุข สอนวิชา นิเทศศาสตร์ ๒๐760
2008 50/35, Alun Amari Road, Bang Yi Khan Subdistrict, Bang Phai District, Bangkok 10700 Thailand
Tel : +66(0) 2422 8899 Fax : +66(0) 2422 8545



of art


Calibration Certificate

Certificate No.: 2502229-001-01
Client name: UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.
Address: 3 Soi Udomsuk 41, Sukhumvit Road,
 Bangchack, Prakanong, Bangkok 10260

Page 1 of 3

Equipment: CHAMBER (Incubator)
Manufacturer: MEMMERT
Model: IPP 260
Serial No.: V615.0187
ID No.: UAE.MIC.003/2559
Order No.: 2502229
Operation No.: 2502229-001
Date of Receipt: 19 March 2025
Date of Calibration: 19 March 2025

Calibrated by Mr.Jerawut Prapawuttipong
 Scientist

Approved by 
 (Mr.Pheraphat Tuanjit) (for)
 Manager, Division of Calibration Laboratory
 Responsible for the Technical Management Team

Date of Issue: 25 March 2025

The uncertainties are for a confidence probability of approximately 95 %.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the National Food Institute.

FCS-009 Revision: 01 Date: 20-04-65



Calibration Report

Certificate No.: 2502229-001-01
Equipment: CHAMBER (Incubator)
 Model: IPP 260 Serial No.: V615.0187
 Resolution: 0.1 °C ID No.: UAE.MIC.003/2559
 Manufacturer: MEMMERT
Date of Calibration: 19 March 2025

Page 2 of 3

Location: LABORATORY, UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.
Environment Condition: Ambient Temperature (16.2 ± 1) °C
 Relative Humidity (32 ± 4) %
 Line Voltage (223 ± 3) Volt

Condition of this results of Calibration:

- This instrument was calibrated by insert 9 standard thermometer into its chamber and calibration according to W-TE-014 Based on TLAS G-20-1/02-08 (E): Guidelines for Calibration and Checks of Temperature Controlled Enclosures.
 - The temperature scale used was based on ITS - 90.
 - All data show below were final values and the initial data may be obtained upon request.

2. Reference Standard Instrument

Instrument	Model	Serial No./ID No.	Certificate No.	Due Date	Through
Digital Thermometer with sensor	34972A	MY49016851	TE 670477-01	4 May 2025	NATIONAL FOOD INSTITUTE
	RTD	CH#101-109/ RTD#101-109			


- This certificate is traceable to International System of Units (SI Units).
- This certificate was certified only for the instrument we calibrated.
- This result of calibration was found accurate as shown on date and place of calibration only.
- Condition of Calibrated item : Good

UUC Description :

Time of Record : Hour 9 Minute - At 35.0 °C
 Fresh air Damper :

Open	Position	-
X Close	Fan	-
-	Not Available	

- Result of Calibration : ☒ Without adjustment ☐ After adjustment


 25 March 2025

FCS-012 Revision: 01 Date: 20-04-65





Equipment : Water Bath
 Condition As-Received : Used Item
 Reference : 2503-0436OC-1

Cert. No.: 25TM501
 Page : 2 of 3

Procedure Used :-

Calibration were conducted using in-house calibration procedure CP-OT04 Based on ASTM E715 according to direct measurement method with Data Acquisition which connected with Industrial Platinum Resistance Thermometer (IPRT).

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

Instrument	Serial No.	Cert. No.	Traceable	Due Date
1) Data Acquisition	MY57013823	23LM71	TPA	12 May 2025

2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certification is traceable to the International System of Unit.


Remark : TPA : Technology Promotion Association (Thailand - Japan)

Result of Calibration :- (*) Without Adjustment

Function of UUC* : Temperature Source

Heat transfer medium used : Water

	Environmental		AC Voltage Supply
	(°C)	(%R.H.)	(Volt)
Beginning of Calibration	24	50	220
Finished of Calibration	25	53	221

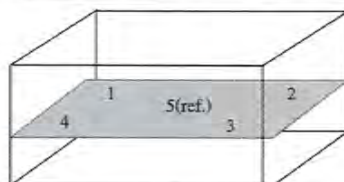

Front

Position :	Ref. Std. S/N.:
1	4804539-006
2	4804539-007
3	4804539-008
4	4804539-009
5(ref.)	4804539-010

เอกสารไม่ควบคุม



Equipment : Water Bath
 Condition As-Received : Used Item
 Reference : 2503-0436OC-1

Cert. No.: 25TM501
 Page : 3 of 3

Result of Calibration :- (*) Without Adjustment

Function of UUC* : Temperature Source

Calibration point (°C)	UUC* Setting (°C)	UUC* Reading (°C)	Average* Standard Reading (°C)					Uncertainty (± °C)
			Position					
			1	2	3	4	5 (ref.)	
44.5	44.4	44.4	44.508	44.531	44.495	44.537	44.510	0.15

Calibration point (°C)	Uniformity (°C)	Stability (± °C)	Coverage Factor <i>k</i>
44.5	0.092	0.048	2

Average* : The average of 30 values in each position.

Uniformity : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.

Stability : One-half of the greatest maximum difference of measured temperature at any one probe.

UUC* : Unit Under Calibration

Note : The reported uncertainty of measurement was included stability and excluded uniformity.

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

เอกสารไม่ควบคุม



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL.0-2717-3000-29 FAX.0-2719-9484



Certificate of Calibration

Cert. No.: 25TM503
Page : 1 of 3

Equipment : Water Bath
Manufacturer : Memmert
Model : WNE 14
Serial No. : L414.1410
ID No. : UAE.MIC.015/2565
Submitted by : United Analyst and Engineering Consultant Co.,Ltd.
3 Soi Udomsuk 41, Sukhumvit Road,
Bangchak, Phrakhanong,
Bangkok 10260
Location : Microbiology Laboratory (302)
Received Order : 19 March 2025
Calibration Date : 19 March 2025
Ambient Temperature : $(26 \pm 10) ^\circ\text{C}$
Relative Humidity : $(50 \pm 30) \%$
AC Line Voltage : $(220 \pm 22) \text{ V}$

Calibrated by : Krisda Malee

Approved by :

Kunchit

Approved Signatory

() Chakrit Waewwanjua
() Suwit Imjai
(✓) Kunchit Promprat

Issue Date : 27 March 2025

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

เอกสารไม่ควบคุม



Equipment : Water Bath
Condition As-Received : Used Item
Reference : 2503-04360C-3
Procedure Used :-

Cert. No.: 25TM503
Page : 2 of 3

Calibration were conducted using in-house calibration procedure CP-OT04 Based on ASTM E715 according to direct measurement method with Data Acquisition which connected with Industrial Platinum Resistance Thermometer (IPRT).

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

Instrument	Serial No.	Cert. No.	Traceable	Due Date
1) Data Acquisition	MY57013823	23LM71	TPA	12 May 2025

2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certification is traceable to the International System of Unit.


Remark : TPA : Technology Promotion Association (Thailand - Japan)

Result of Calibration :- (*) Without Adjustment

Function of UUC* : Temperature Source

Heat transfer medium used : Water

	Environmental		AC Voltage Supply
	(°C)	(%R.H.)	(Volt)
Beginning of Calibration	24	51	221
Finished of Calibration	25	52	220

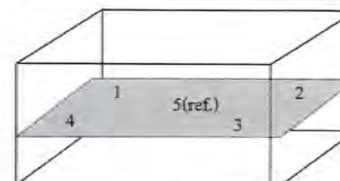

Front

Position :	Ref. Std. S/N.:
1	4804539-006
2	4804539-007
3	4804539-008
4	4804539-009
5(ref.)	4804539-010

เอกสารไม่ควบคุม



Equipment : Water Bath
 Condition As-Received : Used Item
 Reference : 2503-0438OC-3
 Result of Calibration :- (*) Without Adjustment
 Function of UUC* : Temperature Source

Cert. No.: 25TM503
 Page : 3 of 3

Calibration point (°C)	UUC* Setting (°C)	UUC* Reading (°C)	Average* Standard Reading (°C)					Uncertainty (± °C)
			Position					
			1	2	3	4	5 (ref.)	
44.5	44.5	44.5	44.533	44.509	44.527	44.518	44.517	0.15

Calibration point (°C)	Uniformity (°C)	Stability (± °C)	Coverage Factor k
44.5	0.057	0.038	2

Average* : The average of 30 values in each position.

Uniformity : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.

Stability : One-half of the greatest maximum difference of measured temperature at any one probe.

UUC* : Unit Under Calibration

Note : The reported uncertainty of measurement was included stability and excluded uniformity.

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-



มูลนิธิสถาบันพัฒนาอุตสาหกรรมอาหาร
 Foundation for Industrial Development National Food Institute
 Food Industrial Laboratory Service Center



Calibration Certificate

Certificate No.: 2502227-001-01
 Client name: UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.
 Address: 3 Soi Udomsuk 41, Sukhumvit Road,
 Bangchack, Prakhong, Bangkok 10260

Page 1 of 3

Equipment: Electronic Balance

Manufacturer: OHAUS

Model: PX623

Serial No.: C236754745

ID No.: UAE.MIC.055/2565

Order No.: 2502227

Operation No.: 2502227-001

Date of Receipt: 19 March 2025

Date of Calibration: 19 March 2025

Calibrated by Mr.Yothin Charoensuk
 Scientist

Approved by *N. Niyombatt*
 (Mr.Pheraphat Tuanjit)
 Manager, Division of Calibration Laboratory
 Responsible for the Technical Management Team


Date of Issue: 25 March 2025

The uncertainties are for a confidence probability of approximately 95%

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the National Food Institute.

FCS-009 Revision: 01 Date: 20-04-65

2008 ถนนสุขุมวิท ซ. 35 หมู่ 3 แขวงคลองตัน เขตคลองเตย กรุงเทพมหานคร 10700
 2008 So.35, Arun Amarin Road, Bang Yi Khan Subdistrict, Bang Phli District, Bangkok 10700
 Tel: +66(0) 2422 8588 Fax: +66(0) 2422 8545



เอกสารไม่ควบคุม

Calibration Report

Certificate No.: 2502227-001-01
Equipment: Electronic Balance
Model: PX523
Serial No.: C236754745
Capacity: 620
Manufacturer: OHAUS
Resolution: 0.001
ID No.: UAE.MIC.055/2565

Date of Calibration: 19 March 2025 Page 2 of 3

Environment Condition: Ambient Temperature: 22.8 ± 0.3 °C Relative Humidity: 51 ± 0.95 %

Place of Calibration: 301, UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.

Condition of Equipment: Good Condition

Condition of This Results of Calibration:

1. Calibration Method: NFI Method W-MA-001 In-House Method based on UKAS Lab 14 : 2019

2. Reference Standards:

Reference Standard	Model	Serial No.	Calibrated By	Certificate No.	Due Date
Standard Weight Class E2	1mg to 200g	8505567572	TCS	M24041005	19 April 2025
Standard Weight Class E2	500g	8505567696	TCS	M24041015	19 April 2025
Instrument	Model	Serial No.	Calibrated By	Certificate No.	Due Date
Thermo-Hygro Meter	608-H1	NFI.BTH 017/23	Quality Reborn	QR25 0542	10 February 2026

3. This certification is traceable to SI UNIT.

4. This certificate was certified only for the instrument we calibrated.

5. This result of calibration was found accurate as shown on date and place of calibration only.

Calibration Results:

1. Repeatability of Reading:


Nominal Value (g)	Standard Deviation of Reading (g)
300	0.00042
600	0.00048

2. Off-Center Error:


A mass of 200 g was placed and moved to various position on pan.

The balance reading obtained is given in the table.


Reading obtained is given in the table.



☐



☒



☐

1	2	3	4	5	6	(Maximum Difference)
(g)	(g)	(g)	(g)	(g)	(g)	(g)
200.002	200.003	200.001	200.001	200.002	200.002	0.001

F-CS-012 Revision: 01 Date: 20-04-65

2008 ซอยสุขุมวิท 36 แขวงคลองเตย เขตคลองเตย กรุงเทพมหานคร 10700
2008 Soi 36, Arun Amarin Road, Bang Yi Khan Subdistrict, Bang Phat District, Bangkok 10700
Tel: +66(0) 2422 8688 Fax: +66(0) 2422 8545

เอกสารไม่ควบคุม
nfi.or.th



Calibration Report

Certificate No.: 2502227-001-01
Equipment: Electronic Balance
Model: PX523
Serial No.: C236754745
Capacity: 620
Manufacturer: OHAUS
Resolution: 0.001
ID No.: UAE.MIC.055/2565

Date of Calibration: 19 March 2025 Page 3 of 3

Calibration Results: (Continued)

Calibration Range: 0-600 g

Calibration Adjustment: Internal Calibration

3. Departure from Nominal Value:

Nominal Value (g)	Standard Value (g)	Average Reading (g)	Correction (g)	Uncertainty (± g)	Coverage Factor k
Unload	0.0000	0.000	0.000	0.00086	2.00
1	1.0000	1.000	0.000	0.00086	2.00
5	5.0000	4.999	0.001	0.00086	2.00
10	10.0000	10.000	0.000	0.00086	2.00
20	20.0000	20.000	0.000	0.00086	2.00
50	50.0000	50.000	0.000	0.00087	2.00
100	100.0001	100.000	0.000	0.00087	2.00
200	200.0001	200.001	-0.001	0.00090	2.00
300	300.0002	300.001	-0.001	0.00094	2.00
400	400.0003	399.999	0.001	0.0011	2.00
500	500.0003	499.999	0.001	0.0011	2.00
600	600.0004	600.000	0.000	0.0012	2.00

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k, providing a level of confidence of approximately 95 %.

----- End -----

F-CS-012 Revision: 01 Date: 20-04-65

2008 ซอยสุขุมวิท 36 แขวงคลองเตย เขตคลองเตย กรุงเทพมหานคร 10700
2008 Soi 36, Arun Amarin Road, Bang Yi Khan Subdistrict, Bang Phat District, Bangkok 10700
Tel: +66(0) 2422 8688 Fax: +66(0) 2422 8545

เอกสารไม่ควบคุม
nfi.or.th




Calibration Certificate

Certificate No.: 2502229-007-01
Client name: UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.
Address: 3 Soi Udomsuk 41, Sukhumvit Road,
 Bangchack, Prakanong, Bangkok 10260

Page 1 of 3

Equipment: Autoclave
Manufacturer: ALP
Model: CL-40L
Serial No.: 808763
ID No.: UAE.MIC.026/2563
Order No.: 2502229
Operation No.: 2502229-007
Date of Receipt: 19 March 2025
Date of Calibration: 19 March 2025

Calibrated by Mr.Jerawut Prapawuttipong
 Scientist

Approved by 
 (Mr.Pheraphat Tuanjit) (for)
 Manager, Division of Calibration Laboratory
 Responsible for the Technical Management Team

Date of Issue: 25 March 2025

The uncertainties are for a confidence probability of approximately 95 %.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the National Food Institute.

F-CS-009 Revision: 01 Date: 20-04-65



Calibration Report

Certificate No.: 2502229-007-01
Equipment: Autoclave
 Model: CL-40L Serial No.: 808763
 Resolution: 0.1 °C ID No.: UAE.MIC.026/2563
 Manufacturer: ALP
Date of Calibration: 19 March 2025

Page 2 of 3

Location: LABORATORY, UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.
Environment Condition: Ambient Temperature (23 ± 1) °C
 Relative Humidity (60 ± 5) %
 Line Voltage (225 ± 1) Volt

Condition of this results of Calibration:

- This instrument was calibrated by insert 3 standard Data loggers with RTD into its autoclave and calibration according to W-TE-018 based on BS 2646-1:2021, Autoclaves for sterilization in laboratories
 Part 1: Design, construction, safety and performance - Specification.
 - The temperature scale used was based on ITS - 90.
 - All data show below were final values and the initial data may be obtained upon request.

2. Reference Standard Instrument :


Instrument	Model	Serial No.	Certificate No.	Due Date	Through
Digital Thermometer with RTD (Data Logger)	HiTemp140-PT	S35646	TE 670370-01	23-Mar-25	NATIONAL FOOD INSTITUTE
	HiTemp140-PT	S33753	TE 670371-01	23-Mar-25	NATIONAL FOOD INSTITUTE
	HiTemp140-PT	S29973	TE 670372-01	23-Mar-25	NATIONAL FOOD INSTITUTE

- This certificate is traceable to International System of Units (SI Units).
- This certificate was certified only for the instrument we calibrated.
- This result of calibration was found accurate as shown on date and place of calibration only.
- This standard does not apply to sterilizers or disinfectors used for medical, dental, pharmaceutical.
- Condition of Calibrated item : Good

UUC Description : Setting program function sterilization : STERILIZE/NORMAL

Time of sterilization 15 Minute At 115.0 and 121.0 °C

8. Result of Calibration :
- | | |
|-------------------------------------|--------------------|
| <input checked="" type="checkbox"/> | Without adjustment |
| <input type="checkbox"/> | After adjustment |


 25 March 2025

F-CS-012 Revision: 01 Date: 20-04-65



Calibration Report

Certificate No.: 2502229-007-01
Equipment: Autoclave
 Model: CL-40L Serial No.: 808763
 Resolution: 0.1 °C ID No.: UAE.MJC.026/2563
 Manufacturer: ALP

Date of Calibration: 19 March 2025
Calibration point: 115.0 and 121.0 °C

Page 3 of 3

Calibration result:

Calibration Condition	Temperature (°C)	Relative Humidity (%)	Line Voltage (Volt)
Min	22.0	55	224
Max	24.0	65	226



Location of sensor:
 - SENS1 = Attached to the top temperature probe, within 10 mm.
 - SENS2 = 50 mm upper half of the chamber.
 - SENS3 = 20 mm chamber door, within 100 mm.

Table 1 : Reporting of Temperature

Calibration Point (°C)	Measured Temperature (°C) @ Sensor No. (Sensor No.2 is REF)			Uncertainty ± (°C)
	Std.# 1	Std.# 2 (Ref)	Std.# 3	
115.0	115.32	115.46	115.22	0.64
121.0	121.31	121.53	121.31	0.64

Table 2 : Reporting of Characterization Result

UUC* Setting (°C)	UUC* Reading				Stability ± (°C)	Uniformity (°C)	Overall Variation (°C)
	Min (°C)	Max (°C)	Average (°C)	MPa			
115.0	115.0	115.1	115.0	0.08	0.11	0.12	0.26
121.0	121.0	121.1	121.0	0.12	0.13	0.15	0.29

Note

The quoted uncertainty include " Stability " and " Loading effect (20% of Uniformity)"

UUC* = Unit Under Calibration


Stability = One-half of the greatest maximum difference of measured temperatures at any one sensors, for at least half an hour after reaching steady state.

Uniformity = The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time.

Overall Variation = The difference of the maximum and minimum measured temperatures throughout observation time.

The report uncertainty of measurement was based on standard uncertainty multiplied by coverage factor k= 2, providing a level of confidence of approximately 95 %.

----- End -----


 25 March 2025

FCS-012 Revision: 01 Date: 20-04-65