

ภาคผนวกที่ 4

---

สรุปเอกสารสอบเทียบอุปกรณ์เครื่องมือ

เอกสารการสอบเทียบเครื่องมือตรวจวัดระดับเสียงในบรรยากาศ



**SMART TECH CALIBRATION & SERVICES CO., LTD.**  
14/506 MOO 3, RANGSIT-NAKHON NAYOK ROAD, LAM PHAK KUT,  
THANYABURI, PATHUM THANI 12113, THAILAND  
Tel. +662-114-3148 Email : stcal.md@gmail.com Website : stc-cal.com



## Certificate of Calibration

**Certificate No.** STCR-2501082-42

**Work Order No.** STCR-2501082

Page 1 of 3

**Customer Name** : CEM Technology Thailand Co., Ltd.  
31/8 Moo.13 Raikhing Sub-district, Samphran District,  
Nakhonpathom, 73210

**Equipment Name** : Sound Level Meter  
**Manufacturer** : Pulsar  
**Model** : 44  
**Serial Number** : PN2297  
**Control Number** : NS-08-001  
**Received Date** : Jan 24, 2025  
**Calibration Date** : Jan 25, 2025  
**Recommended Due Date** : Jan 25, 2026  
**Calibration Method** : Calibration Procedure No. CPE-04-01

### Environmental Conditions

**Ambient Temperature** :  $(25 \pm 2) ^\circ\text{C}$   
**Ambient Relative Humidity** :  $(50 \pm 15) \% \text{RH}$   
**Calibration Place** : Permanent Calibration Laboratory

**Condition as received** : Normal

**Calibration Result** : See data attached

1. The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor  $k = 2$ , providing a level of confidence of approximately 95%.
2. The Unit Under Calibration (UUC) has been calibrated by using the working standard which is traceable to SI-Units. The calibration procedure documented is intended to implement the requirements of ISO/IEC 17025 : 2017
3. The working standard is indicated in page 2 of this certificate.
4. This report applies to the item calibrated and shall not be reproduced except in full, without written approval by Calibration Laboratory, Smart Tech Calibration & Services Co., Ltd.
5. This results of this report only to the items calibrated.

**Date of Issue** : Jan 29, 2025

**Calibrated by** : Y. Perapon

**Approved by :**



(Mr. Chayut Wongleang)  
Laboratory Manager



@smarttechcal



# Calibration Report

Smart Tech Calibration & Services Co., Ltd.

Certificate No.: STCR-2501082-42

Page 2 of 3

## Standards Equipment Used

Equipment Name	Serial No.	Certificate No.	Due Date	Traceability to
Sound Calibrator	N975185	5523631031354566	Nov 6, 2025	MP-TH

## Traceability

This calibration is traceable to the International System of Unit via :

- MP-TH : Micro Precision Calibration Laboratory (Thailand) Co., Ltd.



# Calibration Report

Smart Tech Calibration & Services Co., Ltd.

Certificate No.: STCR-2501082-42

Page 3 of 3

UUC Range : (30 to 130) dB

Resolution : 0.1 dB

Results of Calibration: [ ] Without adjustment [ ☒ ] With adjustment

Appearance and Function of Use Inspection : NOT GOOD

Sound Level Calibration @ Frequency 1 kHz

Select : A

Response times	STD. Value	UUC. Reading		Correction	(±) Uncertainty
		Before Adjustment	After Adjustment		
FAST	94.09 dB	81.5 dB	-	12.59 dB	0.40 dB
	114.07 dB	111.3 dB	-	2.77 dB	0.40 dB
SLOW	94.09 dB	81.6 dB	-	12.49 dB	0.40 dB
	114.07 dB	111.5 dB	-	2.57 dB	0.40 dB

STD = Standard

UUC = Unit Under Calibration

- End of Certificate -





**SMART TECH CALIBRATION & SERVICES CO., LTD.**  
14/506 MOO 3, RANGSIT-NAKHON NAYOK ROAD, LAM PHAK KUT,  
THANYABURI, PATHUM THANI 12110, THAILAND  
Tel. +662-114-3148 Email : stcal.mtc@gmail.com Website : stc-cal.com



## Certificate of Calibration

**Certificate No.** STCR-2501082-44

**Work Order No.** STCR-2501082

Page 1 of 3

**Customer Name** : CEM Technology Thailand Co., Ltd.  
31/8 Moo.13 Rakkhing Sub-district, Samphran District,  
Nakhonpathom, 73210

**Equipment Name** : Sound Level Meter  
**Manufacturer** : Pulsar  
**Model** : 44  
**Serial Number** : PN2362  
**Control Number** : NS-08-004  
**Received Date** : Jan 24, 2025  
**Calibration Date** : Jan 25, 2025  
**Recommended Due Date** : Jan 25, 2026  
**Calibration Method** : Calibration Procedure No. CPE-04-01

**Environmental Conditions**  
**Ambient Temperature** :  $(25 \pm 2) ^\circ\text{C}$   
**Ambient Relative Humidity** :  $(50 \pm 15) \% \text{RH}$   
**Calibration Place** : Permanent Calibration Laboratory

**Condition as received** : Normal

**Calibration Result** : See data attached

1. The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor  $k = 2$ , providing a level of confidence of approximately 95%.
2. The Unit Under Calibration (UUC) has been calibrated by using the working standard which is traceable to SI-Units. The calibration procedure documented is intended to implement the requirements of ISO/IEC 17025 : 2017
3. The working standard is indicated in page 2 of this certificate.
4. This report applies to the item calibrated and shall not be reproduced except in full, without written approval by Calibration Laboratory, Smart Tech Calibration & Services Co., Ltd.
5. This results of this report only to the items calibrated.

**Date of Issue** : Jan 29, 2025

**Calibrated by** : Y. Perapon

**Approved by :**



@smarttechcal

## Calibration Report

Smart Tech Calibration & Services Co., Ltd.

**Certificate No.:** STCR-2501082-44

Page 2 of 3

### Standards Equipment Used

<u>Equipment Name</u>	<u>Serial No.</u>	<u>Certificate No.</u>	<u>Due Date</u>	<u>Traceability to</u>
Sound Calibrator	N975185	5523631031354566	Nov 6, 2025	MP-TH

### Traceability

This calibration is traceable to the International System of Unit via :

- MP-TH : Micro Precision Calibration Laboratory (Thailand) Co., Ltd.



# Calibration Report

Smart Tech Calibration & Services Co., Ltd

Certificate No.: STCR-2501082-44

Page 3 of 3

UUC Range : (30 to 130) dB Resolution : 0.1 dB

Results of Calibration: [ ] Without adjustment [ ✓ ] With adjustment

Appearance and Function of Use Inspection : GOOD

Sound Level Calibration @ Frequency 1 kHz Select : A

Response times	STD. Value	UUC. Reading		Correction	(±) Uncertainty
		Before Adjustment	After Adjustment		
FAST	94.09 dB	94.8 dB	94.0 dB	0.09 dB	0.40 dB
	114.07 dB	114.8 dB	114.0 dB	0.07 dB	0.40 dB
SLOW	94.09 dB	94.8 dB	94.0 dB	0.09 dB	0.40 dB
	114.07 dB	114.8 dB	114.0 dB	0.07 dB	0.40 dB

STD = Standard

UUC = Unit Under Calibration

- End of Certificate -



SMART TECH CALIBRATION & SERVICES CO., LTD.

14/506 MOO 3, RANGSIT-NAKHON NAYOK ROAD, LAM PHAK KUT,  
THANYABURI, PATHUM THANI 12110, THAILAND

Tel. +662-114-3148 Email : stcal.m@gmail.com Website : stc-cal.com



## Certificate of Calibration

Certificate No. STCR-2501082-52

Work Order No. STCR-2501082

Page 1 of 3

Customer Name : CEM Technology Thailand Co., Ltd.  
31/8 Moo.13 Raikhing Sub-district, Samphran District,  
Nakhonpathom, 73210

Equipment Name : Sound Level Meter  
Manufacturer : Scarlet Tech  
Model : ST-25D  
Serial Number : 10340895  
Control Number : NS-09-007  
Received Date : Jan 24, 2025  
Calibration Date : Jan 25, 2025  
Recommended Due Date : Jan 25, 2026  
Calibration Method : Calibration Procedure No. CPE-04-01

Environmental Conditions  
Ambient Temperature : (25 ± 2) °C  
Ambient Relative Humidity : (50 ± 15) %RH  
Calibration Place : Permanent Calibration Laboratory

Condition as received : Normal

Calibration Result : See data attached

- The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor  $k = 2$ , providing a level of confidence of approximately 95%.
- The Unit Under Calibration (UUC) has been calibrated by using the working standard which is traceable to SI-Units. The calibration procedure documented is intended to implement the requirements of ISO/IEC 17025 : 2017
- The working standard is indicated in page 2 of this certificate.
- This report applies to the item calibrated and shall not be reproduced except in full, without written approval by Calibration Laboratory, Smart Tech Calibration & Services Co., Ltd.
- This results of this report only to the items calibrated.

Date of Issue : Jan 29, 2025

Calibrated by : Y. Perapon

Approved by :





# Calibration Report

Smart Tech Calibration & Services Co., Ltd.

Certificate No.: STCR-2501082-52

Page 2 of 3

## Standards Equipment Used

<u>Equipment Name</u>	<u>Serial No.</u>	<u>Certificate No.</u>	<u>Due Date</u>	<u>Traceability to</u>
Sound Calibrator	N975185	5523631031354566	Nov 6, 2025	MP-TH

## Traceability

This calibration is traceable to the International System of Unit via :

- MP-TH : Micro Precision Calibration Laboratory (Thailand) Co., Ltd.



# Calibration Report

Smart Tech Calibration & Services Co., Ltd.

Certificate No.: STCR-2501082-52

Page 3 of 3

UUC Range : (28 to 133) dB Resolution : 0.1 dB

Results of Calibration: [ ] Without adjustment [ ☒ ] With adjustment

Appearance and Function of Use Inspection : GOOD

Sound Level Calibration @ Frequency 1 kHz Select : A

Response times	STD. Value	UUC. Reading		Correction	(±) Uncertainty
		Before Adjustment	After Adjustment		
FAST	94.09 dB	87.5 dB	94.0 dB	0.09 dB	0.40 dE
	114.07 dB	108.1 dB	114.2 dB	-0.13 dB	0.40 dE
SLOW	94.09 dB	87.5 dB	94.0 dB	0.09 dB	0.40 dE
	114.07 dB	108.1 dB	114.2 dB	-0.13 dB	0.40 dE

Sound Level Calibration @ Frequency 1 kHz Select : C

Response times	STD. Value	UUC. Reading		Correction	(±) Uncertainty
		Before Adjustment	After Adjustment		
FAST	94.09 dB	87.6 dB	94.0 dB	0.09 dB	0.40 dE
	114.07 dB	108.0 dB	114.3 dB	-0.23 dB	0.40 dE
SLOW	94.09 dB	87.6 dB	94.0 dB	0.09 dB	0.40 dE
	114.07 dB	108.0 dB	114.2 dB	-0.13 dB	0.40 dE

STD = Standard

UUC = Unit Under Calibration

- End of Certificate -





**SMART TECH CALIBRATION & SERVICES CO., LTD.**  
14/506 MOO 3, RANGSIT-NAKHON NAYOK ROAD, LAM PHAK KUT,  
THANYABURI, PATHUM THANI 12110, THAILAND  
Tel. +662-114-3148 Email : stcal.md@gmail.com Website : stc-csl.com



## Certificate of Calibration

Certificate No. STCR-2501082-54

Work Order No. STCR-2531082

Page 1 of 3

**Customer Name** : CEM Technology Thailand Co., Ltd.  
31/8 Moo.13 Raikhing Sub-district, Samphran District,  
Nakhonpathom, 73210

**Equipment Name** : Sound Level Meter  
**Manufacturer** : Scarlet Tech  
**Model** : ST-25D  
**Serial Number** : 10340899  
**Control Number** : NS-09-010  
**Received Date** : Jan 24, 2025  
**Calibration Date** : Jan 25, 2025  
**Recommended Due Date** : Jan 25, 2026  
**Calibration Method** : Calibration Procedure No. CPE-04-01

**Environmental Conditions**  
**Ambient Temperature** :  $(25 \pm 2) ^\circ\text{C}$   
**Ambient Relative Humidity** :  $(50 \pm 15) \% \text{RH}$   
**Calibration Place** : Permanent Calibration Laboratory

**Condition as received** : Normal

**Calibration Result** : See data attached

1. The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor  $k = 2$ , providing a level of confidence of approximately 95%.
2. The Unit Under Calibration (UUC) has been calibrated by using the working standard which is traceable to SI-Units. The calibration procedure documented is intended to implement the requirements of ISO/IEC 17025 : 2017
3. The working standard is indicated in page 2 of this certificate.
4. This report applies to the item calibrated and shall not be reproduced except in full, without written approval by Calibration Laboratory, Smart Tech Calibration & Services Co., Ltd.
5. This results of this report only to the items calibrated.

**Date of Issue** : Jan 29, 2025

**Calibrated by** : Y. Perapon

**Approved by :**



@smarttechcal

## Calibration Report

Smart Tech Calibration & Services Co., Ltd.

Certificate No.: STCR-2501082-54

Page 2 of 3

### Standards Equipment Used

Equipment Name	Serial No.	Certificate No.	Due Date	Traceability to
Sound Calibrator	N975185	5523631031354566	Nov 6, 2025	MP-TH

### Traceability

This calibration is traceable to the International System of Unit via :  
- MP-TH : Micro Precision Calibration Laboratory (Thailand) Co., Ltd.





# Calibration Report

Smart Tech Calibration & Services Co., Ltd.

Certificate No.: STCR-2501082-54

Page 3 of 3

UUC Range : (28 to 133) dB

Resolution : 0.1 dB

Results of Calibration: [ ] Without adjustment [ ☒ ] With adjustment

Appearance and Function of Use Inspection : GOOD

Sound Level Calibration @ Frequency 1 kHz Select : A

Response times	STD. Value	UUC. Reading		Correction	(±) Uncertainty
		Before Adjustment	After Adjustment		
FAST	94.09 dB	69.8 dB	94.0 dB	0.09 dB	0.40 dB
	114.07 dB	89.7 dB	113.9 dB	0.17 dB	0.40 dB
SLOW	94.09 dB	69.8 dB	94.0 dB	0.09 dB	0.40 dB
	114.07 dB	89.8 dB	113.9 dB	0.17 dB	0.40 dB

Sound Level Calibration @ Frequency 1 kHz Select : C

Response times	STD. Value	UUC. Reading		Correction	(±) Uncertainty
		Before Adjustment	After Adjustment		
FAST	94.09 dB	69.8 dB	94.0 dB	0.09 dB	0.40 dB
	114.07 dB	89.7 dB	113.9 dB	0.17 dB	0.40 dB
SLOW	94.09 dB	69.8 dB	94.0 dB	0.09 dB	0.40 dB
	114.07 dB	89.8 dB	114.0 dB	0.07 dB	0.40 dB

STD = Standard

UUC = Unit Under Calibration

- End of Certificate -



SMART TECH CALIBRATION & SERVICES CO., LTD.

14/506 MOO 3, RANGSIT-NAKHON NAYOK ROAD, LAM PHAK KUT,

THANYABURI PATHUM THANI 12110, THAILAND

Tel. +662-114-3148 Email : stcal.md@gmail.com Website : stc-cal.com



## Certificate of Calibration

Certificate No. STCR-2509019-6

Work Order No. STCR-2509019

Page 1 of 3

**Customer Name** : CEM Technology Thailand Co., Ltd.  
31/8 Moo.13 Raikhing Sub-district, Samphran District,  
Nakhonpathom, 73210

**Equipment Name** : Sound Level Meter  
**Manufacturer** : SOUNDTEK  
**Model** : ST-109R  
**Serial Number** : 221201934  
**Control Number** : NS-11-001  
**Received Date** : Sep 1, 2025  
**Calibration Date** : Sep 8, 2025  
**Recommended Due Date** : Sep 8, 2026  
**Calibration Method** : Calibration Procedure No. CPE-04-01

### Environmental Conditions

**Ambient Temperature** : (25 ± 2) °C  
**Ambient Relative Humidity** : (50 ± 15) %RH  
**Calibration Place** : Permanent Calibration Laboratory

**Condition as received** : Normal

**Calibration Result** : See data attached

- The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor  $k = 2$ , providing a level of confidence of approximately 95%.
- The Unit Under Calibration (UUC) has been calibrated by using the working standard which is traceable to SI-Units. The calibration procedure documented is intended to implement the requirements of ISO/IEC 17025 : 2017
- The working standard is indicated in page 2 of this certificate.
- This report applies to the item calibrated and shall not be reproduced except in full, without written approval by Calibration Laboratory, Smart Tech Calibration & Services Co., Ltd.
- This results of this report only to the items calibrated.

**Date of Issue** : Sep 11, 2025

**Calibrated by** : Y. Perapon

**Approved by :**

( Mr. Chayut Wongleang )  
Laboratory Manager



@smarttechcal

# Calibration Report

Smart Tech Calibration & Services Co., Ltd.

Certificate No.: STCR-2509019-6

Page 2 of 3

## Standards Equipment Used

Equipment Name	Serial No.	Certificate No.	Due Date	Traceability to
Sound Calibrator	N975185	5523631031354566	Nov 6, 2025	MP-TH

## Traceability

This calibration is traceable to the International System of Unit via :  
- MP-TH : Micro Precision Calibration Laboratory (Thailand) Co., Ltd.



# Calibration Report

Smart Tech Calibration & Services Co., Ltd.

Certificate No.: STCR-2509019-6

Page 3 of 3

UUC Range : (30 to 130) dB Resolution : 0.1 dB

Results of Calibration: [ ] Without adjustment [ ☒ ] With adjustment

Appearance and Function of Use Inspection : GOOD

Sound Level Calibration @ Frequency 1 kHz Select : A

Response times	STD. Value	UUC. Reading		Correction	(±) Uncertainty
		Before Adjustment	After Adjustment		
FAST	94.09 dB	90.1 dB	94.2 dB	-0.11 dB	0.40 dB
	114.07 dB	109.9 dB	114.0 dB	0.07 dB	0.40 dB
SLOW	94.09 dB	90.1 dB	94.2 dB	-0.11 dB	0.40 dB
	114.07 dB	109.9 dB	114.0 dB	0.07 dB	0.40 dB

Sound Level Calibration @ Frequency 1 kHz Select : C

Response times	STD. Value	UUC. Reading		Correction	(±) Uncertainty
		Before Adjustment	After Adjustment		
FAST	94.09 dB	90.1 dB	94.1 dB	-0.01 dB	0.40 dB
	114.07 dB	109.8 dB	114.0 dB	0.07 dB	0.40 dB
SLOW	94.09 dB	90.1 dB	94.1 dB	-0.01 dB	0.40 dB
	114.07 dB	109.8 dB	114.0 dB	0.07 dB	0.40 dB

STD = Standard

UUC = Unit Under Calibration

- End of Certificate -





ELECTRICAL AND ELECTRONICS INSTITUTE  
FOUNDATION FOR INDUSTRIAL DEVELOPMENT

975 Moo 4, Bangpoo Industrial Estate, Soi 8, Sukhumvit Road km 37,  
Phraek Sa, Mueang Samut Prakan, Samut Prakan 10280  
Tel: +66 2709 4860 Fax: +66 2324 0917



Certificate No.: CP20250254EA  
Operation No.: CP2025080247

## Certificate of Calibration

Equipment: Sound Level Meter

Manufacturer: SCARLET TECH

Model/Type: ST11D (Meter), AWA14425 (Microphone), - (Preamplifier)

Serial No.: 820388 (Meter), 79928 (Microphone), - (Preamplifier)

ID No.: NS-12-001

Customer: C.E.M. Technology (Thailand) Co.,Ltd.

Address: 31/8 Moo 13, T.Rai Khing, A.Sam Phran,  
Nakhon Pathom 73210

Received Date: 26 August 2025

Calibrated Date: 2 - 3 September 2025

Issued Date: 4 September 2025

Calibrated by: Ms. Juntaporn Kunhakom

Approved by: \_\_\_\_\_

( Mr. Sittichai Swaksuriyawong )  
Group Manager

This report was prepared electronically using applicable electronic signature. Printing or copy of file are considered as a copy of the document.

The reported uncertainty of measurement was based on standard uncertainty multiplied by a coverage factor ( $k$ ) providing a level of confidence of approximately 95%. This certificate may not be reproduced other than in full except with the prior written approval of the Electrical and Electronics Institute, Foundation for Industrial Development.



ELECTRICAL AND ELECTRONICS INSTITUTE  
FOUNDATION FOR INDUSTRIAL DEVELOPMENT

Certificate No.: CP20250254EA

## Calibration Report

Equipment: Sound Level Meter  
Manufacturer: SCARLET TECH  
Model/Type: ST11D (Meter), AWA14425 (Microphone), - (Preamplifier)  
Serial No.: 820388 (Meter), 79928 (Microphone), - (Preamplifier)  
ID No.: NS-12-001  
Ambient Temperature: ( 23 ± 2 ) °C  
Relative Humidity: ( 50 ± 15 ) %  
Pressure: (101.3 ± 1.5) kPa

Method of Calibration :-  
IEC 61672-3:2013.

### Condition of this result of calibration

1. Reference standards instrument :-

	Instrument	Model	Serial No.	Cert. No.	Due Date
1)	Standard microphone	4180	2661000	AA-1011-25	24 June 2026
2)	Arbitrary Function Generator	AFG2021	C010063	CK20250037EA	25 June 2026
3)	Programmable Attenuator	PA5	2755	EF-0035-24	28 October 2025
4)	6.5 Digit precision multimeter	8846A	9610014	CB20240215EA	26 November 2025
5)	Pressure humidity and Temperature Transmitter	PTU301	F0640003	CL1-P250034 CD20250096EA	10 April 2026 29 March 2026
6)	Performance Audio Analyzer	U8903B	MY56510003	CB20250030EA CK20240069EA	13 February 2026 19 September 2025

2. This result of calibration was found accurate as shown on date and place of calibration only.

3. This certification is traceable to the international system of unit maintained at :-

Reference standards instrument for Acoustic function  
- National Institute of Metrology (Thailand)

Reference standards instrument for Electrical function  
- National Institute of Metrology (Thailand)

- Electrical and Electronics Institute; NSC Accredited Calibration No.0119

- IRPC Metrology Center, IRPC Public Co., Ltd.; NSC Accredited Calibration No.0204.

### Result of Calibration:-

Function : 1. Indication at the calibration check frequency

Reference Acoustic Signal (dB)	Measured value (dB)	Deviation (dB)	Acceptance limits (dB)
-	-	-	-

Certificate No.: CP20250254EA

### Calibration Report

Function : 2. Self-generated Noise

2.1 Microphone Installed

Measured value (dB)
15.7

2.2 Microphone replaced by the electrical input signal device

Frequency Weighting	Measured value (dB)
A-weighting	11.0
C-weighting	12.1
Z-weighting	14.8

Function : 3. Acoustical signal tests of frequency weightings (Without Windscreen)

Meter free-field acoustic response at a level of 84 dB.

Frequency (Hz)	Deviation from various Frequency Weighting Response Curve			
	C-Weighting (dB)	A-Weighting (dB)	Z-Weighting (dB)	Acceptance limits (dB)
125	0.4	0.3	0.4	±1.0
1000	0.0	0.0	0.0	±0.7
8000	0.0	0.1	-0.1	+1.5; -2.5

Function : 4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various Frequency Weighting Response Curve			
	C-Weighting (dB)	A-Weighting (dB)	Z-Weighting (dB)	Acceptance limits (dB)
63	0.0	-0.1	0.0	±1.0
125	0.0	-0.2	0.0	±1.0
250	0.0	-0.1	-0.1	±1.0
500	0.0	-0.1	0.0	±1.0
1000	0.0	0.0	0.0	±0.7
2000	0.1	0.0	-0.1	±1.0
4000	0.1	-0.1	0.0	±1.0
8000	-0.1	-0.1	0.0	+1.5; -2.5
16000	-5.3	-5.2	0.1	+2.5; -16.0

Certificate No.: CP20250254EA

### Calibration Report

Function : 5. Frequency and time weighting at 1 kHz

5.1 Frequency weighting at 1 kHz

Frequency Weighting	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
C-weighting	94.0	0.0	±0.2
A-weighting	94.0	0.0	±0.2
Z-weighting	93.9	-0.1	±0.2

5.2 Time weighting at 1 kHz

Time Weighting	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
Fast	94.0	0.0	±0.1
Slow	94.0	0.0	±0.1
LAeq	94.0	0.0	±0.1

Function : 6. Long-Term Stability

Long-term stability over 30 minutes, with steady 1 kHz signal at reference level.

Time Period to Apply Signal (min)	Reference SPL (dB)	Record SPL at Conclusion of Time Period (dB)	Deviated value (dB)	Acceptance limits (dB)
30	94.0	94.0	0.0	±0.1

Function : 7. Level Linearity on the reference level range

7.1 Level Linearity on the reference level range, Upper

Anticipated Value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
94.0	94.0	0.0	±0.8
99.0	99.0	0.0	±0.8
104.0	104.0	0.0	±0.8
109.0	109.0	0.0	±0.8
114.0	114.0	0.0	±0.8
119.0	119.0	0.0	±0.8
124.0	124.0	0.0	±0.8
129.0	129.0	0.0	±0.8
134.0	134.0	0.0	±0.8
139.0	139.0	0.0	±0.8
140.0	140.0	0.0	±0.8

7.2 Level Linearity on the reference level range, Lower

Anticipated Value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
94.0	94.0	0.0	±0.8
89.0	89.0	0.0	±0.8
84.0	84.0	0.0	±0.8
79.0	79.0	0.0	±0.8
74.0	74.0	0.0	±0.8

Certificate No.: CP20250254EA

### Calibration Report

7.2 Level Linearity on the reference level range, Lower (Cont.)

Anticipated Value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
69.0	69.0	0.0	±0.8
64.0	64.0	0.0	±0.8
59.0	59.0	0.0	±0.8
54.0	54.0	0.0	±0.8
49.0	49.0	0.0	±0.8
44.0	44.0	0.0	±0.8
39.0	39.0	0.0	±0.8
34.0	33.9	-0.1	±0.8
29.0	28.9	-0.1	±0.8
28.0	27.9	-0.1	±0.8
27.0	26.9	-0.1	±0.8
26.0	26.0	0.0	±0.8
25.0	25.0	0.0	±0.8

Function : 8. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
Fast	200	135.9	-0.1	±0.5
	2	118.7	-0.3	+1.0 ; -1.5
	0.25	109.5	-0.5	+1.0 ; -3.0
Slow	200	129.5	-0.1	±0.5
	2	109.9	-0.1	+1.0 ; -3.0
SEL	200	130.0	0.0	±0.5
	2	110.0	0.0	+1.0 ; -1.5
	0.25	100.8	-0.2	+1.0 ; -3.0

Function : 9. Peak C sound level

Number of cycles in test signal	Anticipated Value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
Complete cycle	135.4	135.2	-0.2	±2.0
Positive half cycle	134.4	134.1	-0.3	±1.0
Negative half cycle	134.4	134.1	-0.3	±1.0

Certificate No.: CP20250254EA

### Calibration Report

Function : 10. Overload indication

Measured value (dB)		Deviated value (dB)	Acceptance limits (dB)
Positive one-half cycle	Negative one-half cycle		
143.0	142.8	-0.2	±1.5

Function : 11. High-Level Stability

High-level stability over 5 minutes, with steady 1 kHz signal, 1 dB below upper boundary.

Time Period to Apply Signal (min)	Reference SPL (dB)	Record SPL at Conclusion of Time Period (dB)	Deviated value (dB)	Acceptance limits (dB)
5	139.0	139.0	0.0	±0.1

Uncertainty of measurement

Function	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1) Indication at the calibration check frequency	0.30	Not applicable
2) Self-generated Noise	0.10	Not applicable
3) Acoustical signal tests of frequency weightings - Free-field sound pressure response level	0.30	0.60 (10Hz to 4kHz) 0.70 (>4kHz to 10kHz)
4) Electrical signal tests of frequency weightings	0.20	0.20
5) Frequency and time weighting at 1 kHz	0.20	0.20
6) Long-Term Stability	0.10	0.10
7) Level Linearity on the reference level range	0.30	0.30
8) Tone burst response	0.20	0.30
9) Peak C sound level	0.20	0.35
10) Overload indication	0.24	0.25
11) High-Level Stability	0.10	0.10

Remarks: 1. Indication at the calibration check frequency can not measured because customer does not provide a sound calibrator.  
2. The acceptance limit is for the deviated value.  
3. Acceptance limits was IEC61672-3:2013 Class 1.  
4. The coverage factor  $k = 2.00$

-- End of Report --





ELECTRICAL AND ELECTRONICS INSTITUTE  
FOUNDATION FOR INDUSTRIAL DEVELOPMENT

975 Moo 4, Bangpoo Industrial Estate, Soi 8, Sukhumvit Road km 37,

Phraek Sa, Mueang Samut Prakan, Samut Prakan 10280

Tel: +66 2709 4863 Fax: +66 2324 0917



Certificate No.: CP20250053EA  
Operation No.: CP2025020040

### Certificate of Calibration

Equipment: Sound Level Meter  
Manufacturer: SCARLET TECH  
Model/Type: ST11D (Meter), AWA14425 (Microphone), - (Preamplifier)  
Serial No.: 820891 (Meter), 60237 (Microphone), - (Preamplifier)  
ID No.: NS-12-002  
Customer: C.E.M. Technology (Thailand) Co.,Ltd.  
Address: 31/8 Moo 13 T.Rai Khung, A.Sam Phran,  
Nakorn Phatom 73210  
Received Date: 31 January 2025  
Calibrated Date: 17 - 19 February 2025  
Issued Date: 24 February 2025  
Calibrated by: Ms. Juntaporn Kunhakom

Approved by: \_\_\_\_\_

( Mr. Sittichai Swaksuriyawong )  
Group Manager

This report was prepared electronically using applicable electronic signature. Printing or copy of file are considered as a copy of the document.

The reported uncertainty of measurement was based on standard uncertainty multiplied by a coverage factor ( $k$ ) providing a level of confidence of approximately 95%. This certificate may not be reproduced other than in full except with the prior written approval of the Electrical and Electronics Institute, Foundation for Industrial Development.



ELECTRICAL AND ELECTRONICS INSTITUTE  
FOUNDATION FOR INDUSTRIAL DEVELOPMENT

Certificate No.: CP20250053EA

### Calibration Report

Equipment: Sound Level Meter  
Manufacturer: SCARLET TECH  
Model/Type: ST11D (Meter), AWA14425 (Microphone), - (Preamplifier)  
Serial No.: 820891 (Meter), 60237 (Microphone), - (Preamplifier)  
ID No.: NS-12-002  
Ambient Temperature: ( 23 ± 2 ) °C  
Relative Humidity: ( 50 ± 15 ) %  
Pressure: (101.3 ± 1.5) kPa

Method of Calibration :-

IEC 61672-3:2013.

#### Condition of this result of calibration

1. Reference standards instrument :-

Instrument	Model	Serial No.	Cert. No.	Due Date
1) Standard microphone	4180	2661000	AA-1007-24	6 June 2025
2) Arbitrary Function Generator	AFG2021	C010063	CK20240048EA	23 June 2025
3) Programmable Attenuator	PA5	2913	EF-0021-24	3 June 2025
4) 6.5 Digit precision multimeter	8846A	9609027	CB20240128EA	31 July 2025
5) Pressure humidity and Temperature Transmitter	PTU301	F0640002	CL1-P240022 CD20240180EA	20 March 2025 7 August 2025
6) Performance Audio Analyzer	U8903B	MY56510003	CB20250030EA CK20240069EA	13 February 2026 19 September 2025

2. This result of calibration was found accurate as shown on date and place of calibration only.

3. This certification is traceable to the international system of unit maintained at :-

- Reference standards instrument for Acoustic function
  - National Institute of Metrology (Thailand)
  - Electrical and Electronics Institute, NSC Accredited Calibration No.0119
- Reference standards instrument for Electrical function
  - National Institute of Metrology (Thailand)
  - Electrical and Electronics Institute, NSC Accredited Calibration No.0119

#### Result of Calibration:-

Function : 1. Indication at the calibration check frequency

Reference Acoustic Signal (dB)	Measured value (dB)	Deviation (dB)	Acceptance limits (dB)
-	-	-	-



ELECTRICAL AND ELECTRONICS INSTITUTE  
FOUNDATION FOR INDUSTRIAL DEVELOPMENT

Certificate No.: CP20250053EA

Calibration Report

Function : 2. Self-generated Noise

2.1 Microphone Installed

Measured value (dB)
5.5

2.2 Microphone replaced by the electrical input signal device

Frequency Weighting	Measured value (dB)
A-weighting	5.6
C-weighting	6.5
Z-weighting	12.2

Function : 3. Acoustical signal tests of frequency weightings (Without Windscreen)

Meter free-field acoustic response at a level of 84 dB.

Frequency (Hz)	Deviation from various Frequency Weighting Response Curve			
	C-Weighting (dB)	A-Weighting (dB)	Z-Weighting (dB)	Acceptance limits (dB)
125	0.2	0.1	0.1	±1.0
1000	0.0	0.1	0.0	±0.7
8000	-1.7	-1.3	-1.5	+1.5; -2.5

Function : 4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various Frequency Weighting Response Curve			
	C-Weighting (dB)	A-Weighting (dB)	Z-Weighting (dB)	Acceptance limits (dB)
63	0.0	0.0	0.0	±1.0
125	0.0	-0.1	0.0	±1.0
250	0.0	-0.1	0.0	±1.0
500	0.1	-0.1	0.0	±1.0
1000	0.0	0.0	0.0	±0.7
2000	0.0	0.0	0.0	±1.0
4000	0.1	0.1	0.0	±1.0
8000	-0.1	-0.1	0.0	+1.5; -2.5
16000	-5.2	-5.2	0.1	+2.5; -16.0



ELECTRICAL AND ELECTRONICS INSTITUTE  
FOUNDATION FOR INDUSTRIAL DEVELOPMENT

Certificate No.: CF20250053EA

Calibration Report

Function : 5. Frequency and time weighting at 1 kHz

5.1 Frequency weighting at 1 kHz

Frequency Weighting	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
C-weighting	94.0	0.0	±0.2
A-weighting	94.0	0.0	±0.2
Z-weighting	93.9	-0.1	±0.2

5.2 Time weighting at 1 kHz

Time Weighting	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
Fast	94.0	0.0	±0.1
Slow	94.0	0.0	±0.1
LAeq	94.0	0.0	±0.1

Function : 6. Long-Term Stability

Long-term stability over 30 minutes, with steady 1 kHz signal at reference level.

Time Period to Apply Signal (min)	Reference SPL (dB)	Record SPL at Conclusion of Time Period (dB)	Deviated value (dB)	Acceptance limits (dB)
30	94.0	94.0	0.0	±0.1

Function : 7. Level Linearity on the reference level range

7.1 Level Linearity on the reference level range, Upper

Anticipated Value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
94.0	94.0	0.0	±0.8
99.0	99.0	0.0	±0.8
104.0	104.0	0.0	±0.8
109.0	109.0	0.0	±0.8
114.0	114.0	0.0	±0.8
119.0	119.0	0.0	±0.8
124.0	124.0	0.0	±0.8
129.0	129.0	0.0	±0.8
134.0	134.0	0.0	±0.8
139.0	139.0	0.0	±0.8
140.0	139.9	-0.1	±0.8

7.2 Level Linearity on the reference level range, Lower

Anticipated Value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
94.0	94.0	0.0	±0.8
89.0	89.0	0.0	±0.8
84.0	84.0	0.0	±0.8
79.0	79.0	0.0	±0.8
74.0	74.0	0.0	±0.8

Certificate No.: CP20250053EA

### Calibration Report

7.2 Level Linearity on the reference level range, Lower (Cont.)

Anticipated Value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
69.0	69.0	0.0	±0.8
64.0	64.0	0.0	±0.8
59.0	59.0	0.0	±0.8
54.0	54.0	0.0	±0.8
49.0	49.0	0.0	±0.8
44.0	44.0	0.0	±0.8
39.0	39.0	0.0	±0.8
34.0	33.8	-0.2	±0.8
29.0	28.8	-0.2	±0.8
28.0	27.8	-0.2	±0.8
27.0	26.8	-0.2	±0.8
26.0	25.8	-0.2	±0.8
25.0	24.7	-0.3	±0.8
24.0	23.7	-0.3	±0.8
23.0	22.7	-0.3	±0.8
22.0	21.5	-0.5	±0.8
21.0	20.5	-0.5	±0.8
20.0	19.3	-0.7	±0.8

Function : 8. Tone burst response

Time Weighting	Tone burst duration, T <sub>b</sub> (ms)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
Fast	200	136.0	0.0	±0.5
	2	118.9	-0.1	+1.0 ; -1.5
	0.25	109.8	-0.2	+1.0 ; -3.0
Slow	200	129.6	0.0	±0.5
	2	109.9	-0.1	+1.0 ; -3.0
SEL	200	130.0	0.0	±0.5
	2	110.0	0.0	+1.0 ; -1.5
	0.25	100.9	-0.1	+1.0 ; -3.0

Function : 9. Peak C sound level

Number of cycles in test signal	Anticipated Value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
Complete cycle	135.4	135.1	-0.3	±2.0
Positive half cycle	134.4	134.1	-0.3	±1.0
Negative half cycle	134.4	134.1	-0.3	±1.0

Certificate No.: CP20250053EA

### Calibration Report

Function : 10. Overload indication

Measured value (dB)		Deviated value (dB)	Acceptance limits (dB)
Positive one-half cycle	Negative one-half cycle		
142.6	142.6	0.0	±1.5

Function : 11. High-Level Stability

High-level stability over 5 minutes, with steady 1 kHz signal, 1 dB below upper boundary.

Time Period to Apply Signal (min)	Reference SPL (dB)	Record SPL at Conclusion of Time Period (dB)	Deviated value (dB)	Acceptance limits (dB)
5	139.0	139.0	0.0	±0.1

Uncertainty of measurement

Function	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1) Indication at the calibration check frequency	0.30	Not applicable
2) Self-generated Noise	0.10	Not applicable
3) Acoustical signal tests of frequency weightings - Free-field sound pressure response level	0.30	0.60 (10Hz to 4kHz) 0.70 (>4kHz to 10kHz)
4) Electrical signal tests of frequency weightings	0.20	0.20
5) Frequency and time weighting at 1 kHz	0.20	0.20
6) Long-Term Stability	0.10	0.10
7) Level Linearity on the reference level range	0.30	0.30
8) Tone burst response	0.20	0.30
9) Peak C sound level	0.20	0.35
10) Overload indication	0.24	0.25
11) High-Level Stability	0.10	0.10

Remarks:

1. Indication at the calibration check frequency can not measured because customer does not provide a sound calibrator.
2. The acceptance limit is for the deviated value.
3. Acceptance limits was IEC61672-3:2013 Class 1.
4. The coverage factor  $k = 2.00$

- - End of Report - -





ELECTRICAL AND ELECTRONICS INSTITUTE  
FOUNDATION FOR INDUSTRIAL DEVELOPMENT

975 Moo 4, Bangpoo Industrial Estate, Soi 8, Sukhumvit Road km 37,

Phraek Sa, Mueang Samut Prakan, Samut Prakan 10280

Tel: +66 2709 4860 Fax: +66 2324 0917



Certificate No.: CP20250054EA  
Operation No.: CP2025020041

### Certificate of Calibration

Equipment: Sound Level Meter  
Manufacturer: SCARLET TECH  
Model/Type: ST11D (Meter), AWA14425 (Microphone), - (Preamplifier)  
Serial No.: 820892 (Meter), 57258 (Microphone), - (Preamplifier)  
ID No.: NS-12-003  
Customer: C.E.M. Technology (Thailand) Co.,Ltd.  
Address: 31/8 Moo 13 T.Rai Khung, A.Sam Phran,  
Nakorn Phatom 73210  
Received Date: 31 January 2025  
Calibrated Date: 18 - 20 February 2025  
Issued Date: 24 February 2025  
Calibrated by: Ms. Juntaporn Kunhakorn

Approved by: \_\_\_\_\_

( Mr. Sittchai Swaksuriyawong )  
Group Manager

This report was prepared electronically using applicable electronic signature. Printing or copy of file are considered as a copy of the document.

The reported uncertainty of measurement was based on standard uncertainty multiplied by a coverage factor (k) providing a level of confidence of approximately 95%. This certificate may not be reproduced other than in full except with the prior written approval of the Electrical and Electronics Institute, Foundation for Industrial Development.



ELECTRICAL AND ELECTRONICS INSTITUTE  
FOUNDATION FOR INDUSTRIAL DEVELOPMENT

Certificate No.: CP20250054EA

### Calibration Report

Equipment: Sound Level Meter  
Manufacturer: SCARLET TECH  
Model/Type: ST11D (Meter), AWA14425 (Microphone), - (Preamplifier)  
Serial No.: 820892 (Meter), 57258 (Microphone), - (Preamplifier)  
ID No.: NS-12-003  
Ambient Temperature: ( 23 ± 2 ) °C  
Relative Humidity: ( 50 ± 15 ) %  
Pressure: (101.3 ± 1.5) kPa

Method of Calibration :-

IEC 61672-3:2013.

Condition of this result of calibration

1. Reference standards instrument :-

Instrument	Model	Serial No.	Cert. No.	Due Date
1) Standard microphone	4180	2661000	AA-1007-24	6 June 2025
2) Arbitrary Function Generator	AFG2021	C010063	CK20240048EA	23 June 2025
3) Programmable Attenuator	PA5	2913	EF-0021-24	3 June 2025
4) 6.5 Digit precision multimeter	8846A	9609027	CB20240128EA	31 July 2025
5) Pressure humidity and Temperature Transmitter	PTU301	F0640002	CL1-P240022 CD20240180EA	20 March 2025 7 August 2025
6) Performance Audio Analyzer	U8903B	MY56510003	CB20250030EA CK20240069EA	13 February 2026 19 September 2025

2. This result of calibration was found accurate as shown on date and place of calibration only.

3. This certification is traceable to the international system of unit maintained at :-

Reference standards instrument for Acoustic function

- National Institute of Metrology (Thailand)

- Electrical and Electronics Institute, NSC Accredited Calibration No.0119

Reference standards instrument for Electrical function

- National Institute of Metrology (Thailand)

- Electrical and Electronics Institute, NSC Accredited Calibration No.0119

### Result of Calibration:-

Function : 1. Indication at the calibration check frequency

Reference Acoustic Signal (dB)	Measured value (dB)	Deviation (dB)	Acceptance limits (dB)
-	-	-	-

Certificate No.: CP20250054EA

### Calibration Report

Function : 2. Self-generated Noise

2.1 Microphone Installed

Measured value (dB)
15.8

2.2 Microphone replaced by the electrical input signal device

Frequency Weighting	Measured value (dB)
A-weighting	7.8
C-weighting	8.2
Z-weighting	14.6

Function : 3. Acoustical signal tests of frequency weightings (Without Windscreen)

Meter free-field acoustic response at a level of 84 dB.

Frequency (Hz)	Deviation from various Frequency Weighting Response Curve			
	C-Weighting (dB)	A-Weighting (dB)	Z-Weighting (dB)	Acceptance limits (dB)
125	0.2	0.1	0.1	±1.0
1000	0.1	0.1	0.1	±0.7
8000	-0.8	-0.8	-0.7	+1.5; -2.5

Function : 4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various Frequency Weighting Response Curve			
	C-Weighting (dB)	A-Weighting (dB)	Z-Weighting (dB)	Acceptance limits (dB)
63	0.1	0.1	0.0	±1.0
125	0.1	-0.1	0.0	±1.0
250	0.0	0.0	0.0	±1.0
500	0.0	0.0	-0.1	±1.0
1000	0.0	0.0	0.0	±0.7
2000	0.1	0.1	-0.1	±1.0
4000	0.1	0.0	0.0	±1.0
8000	0.0	0.0	-0.1	+1.5; -2.5
16000	-5.2	-5.1	-0.1	+2.5; -16.0

Certificate No.: CF20250054EA

### Calibration Report

Function : 5. Frequency and time weighting at 1 kHz

5.1 Frequency weighting at 1 kHz

Frequency Weighting	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
C-weighting	94.0	0.0	±0.2
A-weighting	94.0	0.0	±0.2
Z-weighting	93.9	-0.1	±0.2

5.2 Time weighting at 1 kHz

Time Weighting	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
Fast	94.0	0.0	±0.1
Slow	94.0	0.0	±0.1
LAeq	94.0	0.0	±0.1

Function : 6. Long-Term Stability

Long-term stability over 30 minutes, with steady 1 kHz signal at reference level.

Time Period to Apply Signal (min)	Reference SPL (dB)	Record SPL at Conclusion of Time Period (dB)	Deviated value (dB)	Acceptance limits (dB)
30	94.0	94.0	0.0	±0.1

Function : 7. Level Linearity on the reference level range

7.1 Level Linearity on the reference level range, Upper

Anticipated Value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
94.0	94.0	0.0	±0.8
99.0	99.0	0.0	±0.8
104.0	104.0	0.0	±0.8
109.0	109.0	0.0	±0.8
114.0	114.0	0.0	±0.8
119.0	119.0	0.0	±0.8
124.0	124.0	0.0	±0.8
129.0	129.0	0.0	±0.8
134.0	134.0	0.0	±0.8
139.0	139.0	0.0	±0.8
140.0	140.0	0.0	±0.8

7.2 Level Linearity on the reference level range, Lower

Anticipated Value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
94.0	94.0	0.0	±0.8
89.0	89.0	0.0	±0.8
84.0	84.0	0.0	±0.8
79.0	79.0	0.0	±0.8
74.0	74.0	0.0	±0.8



Certificate No.: CP20250054EA

### Calibration Report

#### 7.2 Level Linearity on the reference level range, Lower (Cont.)

Anticipated Value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
69.0	69.0	0.0	±0.8
64.0	64.0	0.0	±0.8
59.0	59.0	0.0	±0.8
54.0	54.0	0.0	±0.8
49.0	49.0	0.0	±0.8
44.0	44.0	0.0	±0.8
39.0	39.0	0.0	±0.8
34.0	33.8	-0.2	±0.8
29.0	28.8	-0.2	±0.8
28.0	27.8	-0.2	±0.8
27.0	26.8	-0.2	±0.8
26.0	25.8	-0.2	±0.8
25.0	24.8	-0.2	±0.8
24.0	23.7	-0.3	±0.8
23.0	22.6	-0.4	±0.8
22.0	21.5	-0.5	±0.8
21.0	20.5	-0.5	±0.8
20.0	19.4	-0.6	±0.8
19.0	18.3	-0.7	±0.8

#### Function : 8. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
Fast	200	136.0	0.0	±0.5
	2	118.8	-0.2	+1.0 ; -1.5
	0.25	109.8	-0.2	+1.0 ; -3.0
Slow	200	129.5	-0.1	±0.5
	2	109.9	-0.1	+1.0 ; -3.0
	200	130.0	0.0	±0.5
SEL	2	110.0	0.0	+1.0 ; -1.5
	0.25	100.9	-0.1	+1.0 ; -3.0

#### Function : 9. Peak C sound level

Number of cycles in test signal	Anticipated Value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
Complete cycle	135.4	135.1	-0.3	±2.0
Positive half cycle	134.4	134.1	-0.3	±1.0
Negative half cycle	134.4	134.1	-0.3	±1.0

Certificate No.: CP20250054EA

### Calibration Report

#### Function : 10. Overload indication

Measured value (dB)		Deviated value (dB)	Acceptance Limits (dB)
Positive one-half cycle	Negative one-half cycle		
143.3	143.5	0.2	±1.5

#### Function : 11. High-Level Stability

High-level stability over 5 minutes, with steady 1 kHz signal, 1 dB below upper boundary.

Time Period to Apply Signal (min)	Reference SPL (dB)	Record SPL at Conclusion of Time Period (dB)	Deviated value (dB)	Acceptance Limits (dB)
5	139.0	139.0	0.0	±0.1

#### Uncertainty of measurement

Function	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1) Indication at the calibration check frequency	0.30	Not applicable
2) Self-generated Noise	0.10	Not applicable
3) Acoustical signal tests of frequency weightings - Free-field sound pressure response level	0.30	0.60 (10Hz to 4kHz) 0.70 (>4kHz to 10kHz)
4) Electrical signal tests of frequency weightings	0.20	0.20
5) Frequency and time weighting at 1 kHz	0.20	0.20
6) Long-Term Stability	0.10	0.10
7) Level Linearity on the reference level range	0.30	0.30
8) Tone burst response	0.20	0.30
9) Peak C sound level	0.20	0.35
10) Overload indication	0.24	0.25
11) High-Level Stability	0.10	0.10

- Remarks:
1. Indication at the calibration check frequency can not measured because customer does not provide a sound calibrator.
  2. The acceptance limit is for the deviated value.
  3. Acceptance limits was IEC61672-3:2013 Class 1.
  4. The coverage factor  $k = 2.00$

-- End of Report --



## CERTIFICATE OF CALIBRATION

NO. 20250104123

Name of Product:	Sound Level Meter
Model:	ST-12D
Serial Number:	10351425
Specification:	Class 1
Conclusion:	Pass
Date of calibration:	2025-03-04
Due Date:	2026-03-03

Calibrated by:

*Chen*



- I. This report certifies that all calibration equipment used in the test is traceable with the internal ISO9001 procedures and meets all specification given in the Manual(s) or respectively surpass then, and applies only to the unit identified above.
- II. This certificate is produced with advanced equipment & procedures which permit comprehensive quality assurance verification of all data supplied herein.
- III. This certificate of calibration shall not be reproduced except in full, without written permission of the Scarlet Tech Co Ltd Taiwan.

1. Preliminary inspection: OK

2. Type & serial No. of Microphone: AWA14423-80567

3. Adjustments to indicated sound levels:

Type of Calibrator B&K 4231

Sound Pressure Level 94.0 dB

Equivalent Free-field Sound Level (reference environment conditions) 93.8 dB

4. Measuring up limit: 140 dBA

5. Frequency weightings (Acoustic signal tests for Z weighting, other electric signal tests.)

Nominal frequency /Hz	Frequency weighting / dB			Nominal frequency /Hz	frequency weighting / dB		
	A	C	Z		A	C	Z
10	-69.6	-14.3	+0.1	1000	0.0	-0.1	0.0
20	-50.3	-6.2	+0.1	2000	+1.3	-0.1	0.0
31.5	-39.5	-3.0	0.0	4000	+1.0	-0.8	0.0
63	-26.2	-0.8	0.0	8000	-1.2	-3.1	0.0
125	-16.2	-0.2	0.0	12500	-6.0	-7.9	-0.9
250	-8.7	0.0	0.0	16000	-12.0	-13.9	0.0
500	-3.2	0.0	0.0	20000	-23.3	-24.4	0.0

### 6. Self-generated noise

Microphone replaced by electrical input signal device

10.1 dB(A)	10.4 dB(C)	16.2 dB(Z)
------------	------------	------------

### 7. F&S Weighting

Rate of the F weighting decrease (dB/s)	33.7
Rate of the S weighting decrease (dB/s)	3.9
Deviation of F&S	0.0

### 8. Level Linearity (A-weighting at frequency 1 kHz)

Reference sound level 90.0 dB

Max error at 10dB steps upper reference sound level 0.1 dB

Max error at 1dB steps within 5dB of the upper limit linear operating range 0.0 dB

Max error at 10dB steps below reference sound level 0.2 dB

Max error at 1dB steps within 5dB upper the lower limit linear operating range 0.2 dB

### 9. Tone burst response (A Weighting) :

Single Toneburst duration /ms	Toneburst response /dB			
	$L_{Fmax}-L_A$	$L_{Amax}-L_A$	$L_A-L_A$	$L_{Aref}-L_A$
500	-0.1	-4.1	-3.0	-7.0
200	-1.0	-7.5	-7.0	-7.0
2	-18.4	-27.1	-27.0	-7.1
0.25	-27.4	/	-36.3	-7.0

### 10. Peak C sound level (500Hz) :

Cycle	One cycle	nominal value	Positive half	nominal value	Negative half	nominal value
$LC_{peak}-LC(dB)$	3.4	3.5	2.3	2.4	2.4	2.4

11. Overload indication: Pass

### 12. Statistical analysis function

Sweep signal maximum indicated sound level: 112.8 dB

Sweep amplitude: 40 dB

Scan cycle time: 60 S; Measurement period: 180 S.

Items	Measured value/dB	Theoretical calculated value/dB	Error/dB
L <sub>Aeq,T</sub>	103.2	103.1	0.1
L <sub>5</sub>	110.8	110.8	0.0
L <sub>10</sub>	108.8	108.8	0.0
L <sub>50</sub>	92.9	92.8	0.1
L <sub>90</sub>	76.9	76.9	0.0
L <sub>95</sub>	75.0	74.9	0.1

Uncertainty of measurement results: 0.4 dB (k=2)

13.Part of sound exposure: Pass

14.Data logging function: Pass

15. SD card & wave recording function: Pass

Environment conditions:

Air temperature: 23 °C  
Relative humidity: 80 %  
Static pressure: 102.0 kPa

Reference equipment used in the calibration:

Description:	Model	Serial No.	Expiry Date	Traceable To
Microphone	B&K 4191	2929405	2025-12-15	NIML
Multi function sound calibrator	B&K 4226	2288444	2025-10-15	CIGISMEC
Signal generator	DS 360	33873	2025-10-15	CEPREI


Test specifications:

1. All Scarlet's Sound level Meter has been calibrated in accordance with the requirements as specified in ISO 17025 and the lab calibration procedure SMTPO04-CA-152.
2. The electrical tests were performed using an electrical signal substituted for the microphone which was removed and replaced by an equivalent capacitance within a tolerance of ±20%.
3. The acoustic calibration was performed using an B&K 4226 sound calibrator and corrections was applied for the difference between the free-field and pressure responses of the Sound Level Meter.

References:

IEC 61672-3 Sound Level Meters Part 3: Periodic tests

เอกสารการสอบเทียบเครื่องมือตรวจวัดคุณภาพอากาศในบรรยากาศ



### Certificate of Analyzer Performance Testing

Calibrated Date : 3-Mar-25 Certificate No. : 0325-001  
Page : 1/1

#### Analyzer Instruments

Analyzer Type : CO Analyzer Manufacturer : Thermo Environmental  
Model : 48C Serial No. : 65775350

#### Environmental

Temperature : 25.6 °C  
Humidity : 42.3 %RH

#### Calibration System

##### Calibrator Units


Gas Calibration : Thermo Environmental Zero Air Generator : API  
Model : 146C Model : 701  
Serial No. : 514811458 Serial No. : 179

#### Standard Gas

NO Conc. : 2 ppm Cylinder No. : 307199  
SO2 Conc. : 2 ppm Expire Date : 10-Oct-25  
CO Conc. : 50 ppm


#### Calibration Check

Gas	Zero			Span		
	Reading Value (ppm)	Expected Value (ppm)	Drift (%)	Reading Value (ppm)	Expected Value (ppm)	Drift (%)
Before						
CO	0.037	0.000	0.04	49.850	50.000	-0.30
After						
CO	0.000	0.000	0.00	50.000	50.000	0.00

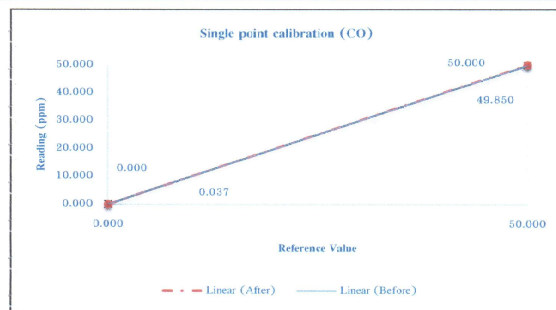

Calibrated by :

*Tong Piima*  
(Mr. Tong Piima)



### Certificate of Analyzer Performance Testing

Calibrated Date : 25-Mar-25 Certificate No. : 0325-004  
Page : 1/1

#### Analyzer Instruments

Analyzer Type : CO Analyzer Manufacturer : Thermo Environmental  
Model : 48C Serial No. : 401304261

#### Environmental

Temperature : 20.8 °C  
Humidity : 46.9 %RH

#### Calibration System

##### Calibrator Units


Gas Calibration : Thermo Environmental Zero Air Generator : API  
Model : 146C Model : 701  
Serial No. : 514811458 Serial No. : 179

#### Standard Gas

NO Conc. : 2 ppm Cylinder No. : 307199  
SO2 Conc. : 2 ppm Expire Date : 10-Oct-25  
CO Conc. : 50 ppm


#### Calibration Check

Gas	Zero			Span		
	Reading Value (ppm)	Expected Value (ppm)	Drift (%)	Reading Value (ppm)	Expected Value (ppm)	Drift (%)
Before						
CO	0.021	0.000	0.02	49.781	50.000	-0.44
After						
CO	0.000	0.000	0.00	50.000	50.000	0.00

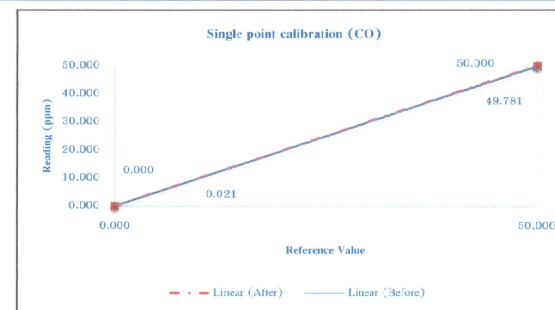

Calibrated by :

*Tong Piima*  
(Mr. Tong Piima)



### Certificate of Analyzer Performance Testing

Calibrated Date : 20-Aug-25 Certificate No. : 0825-007  
Page : 1/1

**Analyzer Instruments**

Analyzer Type : CO Analyzer Manufacturer : Thermo Environmental  
Model : 48C Serial No. : 508011064

**Environmental**

Temperature : 22.4 °C  
Humidity : 40.5 %RH

**Calibration System**

**Calibrator Units**


Gas Calibration : Thermo Environmental Zero Air Generator : API  
Model : 146C Model : 701  
Serial No. : 514811458 Serial No. : 179

**Standard Gas**

NO Conc. : 2 ppm Cylinder No. : 307199  
SO<sub>2</sub> Conc. : 2 ppm Expire Date : 10-Oct-25  
CO Conc. : 50 ppm


#### Calibration Check

Gas	Zero			Span		
	Reading Value (ppm)	Expected Value (ppm)	Drift (%)	Reading Value (ppm)	Expected Value (ppm)	Drift (%)
Before						
CO	0.079	0.000	0.08	50.1	50.000	0.20
After						
CO	0.000	0.000	0.00	50.0	50.000	0.00

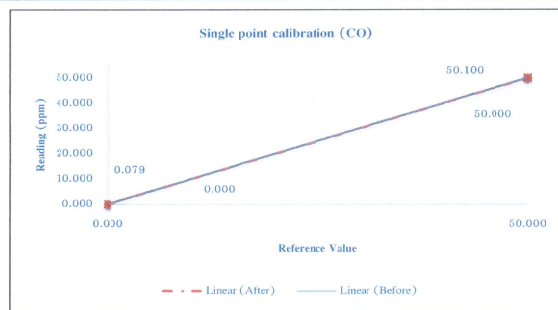

Calibrated by :

*Tong Puima*  
(M/Tong Puima)



### TSP High Volume Sampler TE-5000 TSP Sampler Verification

#### Site Information

Location: - Site ID: - Date: 21 Dec 24  
Sampler: TE-5000 TSP Serial No: 3262 Tech: Tong.P

#### Site Conditions

Barometric Pressure (in Hg): 27.90 Corrected Pressure (mm Hg): 708.7  
Temperature (deg F): 75.4 Temperature (deg K): 297.3  
Average Press. (in Hg): 26.00 Corrected Average (mm Hg): 660.4  
Average Temp (Deg F): 74.6 Average Temp: (Deg K): 296.8

#### Calibration Orifice

Make: Tisch Qstd Slope: 1.58304  
Model: TE-5028A Qstd Intercept: -0.01520  
Serial #: 1179 Calibration Due Date 10 December 2025

#### Calibration Information

Plate or Test #	H2O (in)	Qstd (m3/min)	I (chart)	IC (corrected)	Linear Regression
1	8.20	1.759	62.9	60.81	Slope: 41.1217
2	6.60	1.579	56.0	54.14	Intercept: -11.0896
3	5.00	1.375	47.8	46.21	Corr. Coeff: 0.9983
4	4.50	1.305	43.9	42.44	
5	3.90	1.216	39.7	38.38	
# of Observations: 5					

#### Calculations

$$Qstd = 1/m[\text{Sqrt}(H_2O(Pa/Pstd)(Tstd/Ta))-b]$$
$$IC = I[\text{Sqrt}(Pa/Pstd)(Tstd/Ta)]$$

Qstd = standard flow rate  
IC = corrected chart response  
I = actual chart response  
m = calibrator Qstd slope  
b = calibrator Qstd intercept  
Ta = actual temperature during calibration (deg K)  
Pa = actual pressure during calibration (mm Hg)  
Tstd = 298 deg K  
Pstd = 760 mm Hg  
For subsequent calculation of sampler flow:  
 $1/m((I)/[\text{Sqrt}(298/Tav)(Pav/760)]-b)$

Enter Average I (chart): 50.1  
Average Flow Calculation m3/min  
1.406730656  
Average Flow Calculation in cfm  
49.67269199  
Sample Time (Hrs): 24.0  
Total flow in 24 hours m3/min  
2025.692144  
Total flow in 24 hours cfm  
71528.67647

NOTE: Ensure calibration orifice has been certified within 12 months of use



# TSP

Trade & Engineering  
TSP High Volume Sampler  
TE-5000 TSP Sampler Verification

## Site Information

Location: -	Site ID: -	Date: 21 Dec 24
Sampler: TE-5000 TSP	Serial No: 3263	Tech: Tong.P

## Site Conditions

Barometric Pressure (in Hg): 27.80	Corrected Pressure (mm Hg): 706.1
Temperature (deg F): 76.0	Temperature (deg K): 297.6
Average Press. (in Hg): 26.30	Corrected Average (mm Hg): 668.0
Average Temp (Deg F): 75.0	Average Temp: (Deg K): 297.0

## Calibration Orifice

Make: Tisch	Qstd Slope: 1.58304
Model: TE-5028A	Qstd Intercept: -0.01520
Serial#: 1179	Calibration Due Date 10 December 2025

## Calibration Information

Plate or Test #	H2O (in)	Qstd (m3/min)	I (chart)	IC (corrected)	Linear Regression
1	6.10	1.514	60.8	58.65	Slope: 31.4134
2	4.30	1.273	54.3	52.38	Intercept: 11.5313
3	3.20	1.100	47.2	45.53	Corr. Coeff: 0.9947
4	2.40	0.954	44.0	42.44	
5	2.00	0.871	39.5	38.10	# of Observations: 5

## Calculations

Qstd =  $1/m[\text{Sqrt}(\text{H2O}(\text{Pa}/\text{Pstd})(\text{Tstd}/\text{Ta})) - b]$   
IC =  $I[\text{Sqrt}(\text{Pa}/\text{Pstd})(\text{Tstd}/\text{Ta})]$

Qstd = standard flow rate  
IC = corrected chart response  
I = actual chart response  
m = calibrator Qstd slope  
b = calibrator Qstd intercept  
Ta = actual temperature during calibration (deg K)  
Pa = actual pressure during calibration (mm Hg)  
Tstd = 298 deg K  
Pstd = 760 mm Hg  
For subsequent calculation of sampler flow:  
 $1/m((I)[\text{Sqrt}(298/\text{Tav})(\text{Pav}/760)] - b)$

Enter Average I (chart): 49.2  
Average Flow Calculation m3/min  
1.102476438  
Average Flow Calculation in cfm  
38.92925225  
Sample Time (Hrs): 24.0  
Total flow in 24 hours m3/min  
1587.566071  
Total flow in 24 hours cfm  
56058.12323

NOTE: Ensure calibration orifice has been certified within 12 months of use

Tisch Environmental 145 South Miami Ave, Cleves OH 45002 • 877.263.7610 • sales@tisch-env.com • www.tisch-env.com

# TSP

Trade & Engineering  
TSP High Volume Sampler  
TE-5000 TSP Sampler Verification

## Site Information

Location: -	Site ID: -	Date: 10 Oct 24
Sampler: TE-5000 TSP	Serial No: 3275	Tech: Tong.P

## Site Conditions

Barometric Pressure (in Hg): 28.20	Corrected Pressure (mm Hg): 716.3
Temperature (deg F): 75.4	Temperature (deg K): 297.3
Average Press. (in Hg): 27.35	Corrected Average (mm Hg): 694.7
Average Temp (Deg F): 75.1	Average Temp: (Deg K): 297.1

## Calibration Orifice

Make: Tisch	Qstd Slope: 1.57894
Model: TE-5028A	Qstd Intercept: -0.01520
Serial#: 1179	Calibration Due Date 10 December 2024

## Calibration Information

Plate or Test #	H2O (in)	Qstd (m3/min)	I (chart)	IC (corrected)	Linear Regression
1	8.45	1.799	62.0	60.27	Slope: 36.0752
2	6.55	1.585	57.8	56.18	Intercept: -3.3857
3	5.40	1.440	50.2	48.80	Corr. Coeff: 0.9866
4	4.70	1.344	44.9	43.64	
5	4.20	1.112	37.9	36.84	# of Observations: 5

## Calculations

Qstd =  $1/m[\text{Sqrt}(\text{H2O}(\text{Pa}/\text{Pstd})(\text{Tstd}/\text{Ta})) - b]$   
IC =  $I[\text{Sqrt}(\text{Pa}/\text{Pstd})(\text{Tstd}/\text{Ta})]$

Qstd = standard flow rate  
IC = corrected chart response  
I = actual chart response  
m = calibrator Qstd slope  
b = calibrator Qstd intercept  
Ta = actual temperature during calibration (deg K)  
Pa = actual pressure during calibration (mm Hg)  
Tstd = 298 deg K  
Pstd = 760 mm Hg  
For subsequent calculation of sampler flow:  
 $1/m((I)[\text{Sqrt}(298/\text{Tav})(\text{Pav}/760)] - b)$

Enter Average I (chart): 50.6  
Average Flow Calculation m3/min  
1.435835729  
Average Flow Calculation in cfm  
50.7004135  
Sample Time (Hrs): 24.0  
Total flow in 24 hours m3/min  
2067.60345  
Total flow in 24 hours cfm  
73008.59544

NOTE: Ensure calibration orifice has been certified within 12 months of use

Tisch Environmental 145 South Miami Ave, Cleves OH 45002 • 877.263.7610 • sales@tisch-env.com • www.tisch-env.com

# TSP

Trade & Engineering  
TSP High Volume Sampler  
TE-5000 TSP Sampler Verification

## Site Information

Location: - Site ID: - Date: 10 Oct 24  
Sampler: TE-5000 TSP Serial No: 3276 Tech: Tong.P

## Site Conditions

Barometric Pressure (in Hg): 28.50 Corrected Pressure (mm Hg): 723.9  
Temperature (deg F): 75.5 Temperature (deg K): 297.3  
Average Press. (in Hg): 27.30 Corrected Average (mm Hg): 693.4  
Average Temp (Deg F): 75.0 Average Temp: (Deg K): 297.0

## Calibration Orifice

Make: Tisch Qstd Slope: 1.57894  
Model: TE-5028A Qstd Intercept: -0.01520  
Serial#: 1179 Calibration Due Date 10 December 2024

## Calibration Information

Plate or Test #	H2O (in)	Qstd (m3/min)	I (chart)	IC (corrected)	Linear Regression
1	8.40	1.803	61.8	60.38	Slope: 36.6686
2	6.50	1.587	56.2	54.91	Intercept: -4.7465
3	5.35	1.441	50.1	48.95	Corr. Coeff: 0.9926
4	4.65	1.344	44.3	43.28	
5	4.25	1.112	36.8	35.96	

# of Observations: 5

## Calculations

$Q_{std} = 1/m[\text{Sqrt}((H2O(Pa/Pstd)(Tstd/Ta)))-b]$   
 $IC = I[\text{Sqrt}(Pa/Pstd)(Tstd/Ta)]$

Qstd = standard flow rate  
IC = corrected chart response  
I = actual chart response  
m = calibrator Qstd slope  
b = calibrator Qstd intercept  
Ta = actual temperature during calibration (deg K)  
Pa = actual pressure during calibration (mm Hg)  
Tstd = 298 deg K  
Pstd = 760 mm Hg  
For subsequent calculation of sampler flow:  
 $1/m[(T)[\text{Sqrt}(298/Tav)(Pav/760)]-b]$

m = sampler slope  
b = sampler intercept  
I = chart response  
Tav = daily average temperature  
Pav = daily average pressure

Enter Average I (chart): 49.8  
Average Flow Calculation m3/min  
1.429841813  
Average Flow Calculation in cfm  
50.48876392  
Sample Time (Hrs): 24.0  
Total flow in 24 hours m3/min  
2058.972211  
Total flow in 24 hours cfm  
72703.82005

NOTE: Ensure calibration orifice has been certified within 12 months of use

Tisch Environmental 145 South Miami Ave, Cleves OH 45002 • 877.263.7610 • sales@tisch-env.com • www.tisch-env.com

# TSP

Trade & Engineering

## PM10 High Volume Sampler Verification

## Site Information

Location: - Site ID: - Date: 23 December 2024  
Sampler: TE-6070 PM10 Serial No: 1629 Tech: Tong P.

## Site Conditions

Barometric Pressure (in Hg): 28.90 Corrected Pressure (mm Hg): 734.1  
Temperature (deg F): 75.5 Temperature (deg K): 297.2  
Average Press. (in Hg): 28.00 Corrected Average (mm Hg): 711.2  
Average Temp. (deg F): 75.5 Average Temp. (deg K): 297.2

## Calibration Orifice

Make: Tisch Environmental, Inc. Qstd Slope: 1.58407  
Model: TE-5028A Qstd Intercept: -0.01510  
Serial#: 1179 Calibration Due Date: 22 Oct 25

## Calibration Data

Plate or Test #	In H2O	Qa (m3/min)	I (chart)	IC (corrected)	Linear Regression
1	7.90	1.138	60.2	38.30	Slope 34.6406
2	6.50	1.034	55.3	35.19	Intercept -0.9094
3	5.10	0.917	49.4	31.43	Corr. Coeff 0.9947
4	4.30	0.842	43.0	27.36	SFR 1.095
5	3.10	0.717	38.0	24.18	SSP 58.18

# of Observations: 5

## Calculations

$Q_a = 1/m(\text{Sqrt}((H2O)(Ta/Pa)))-b)$   
 $IC = I(\text{Sqrt}(Ta/Pa))$

$SFR = 1.13(Ps/Pa)(Ta/Ts)$   
 $SSP = (m*SFR+b)(\text{Sqrt}(Pa/Ta))$

m = sampler slope  
b = sampler intercept  
I = chart response  
Tav = daily average temperature  
Pav = daily average pressure

Qa = actual flow rate  
IC = corrected chart response  
m = calibrator slope  
b = calibrator intercept  
Ta = actual temperature (deg K)  
Pa = actual pressure (mm Hg)  
For subsequent calculation of sampler flow:

SFR = sampler set point flow rate  
SSP = sampler chart set point  
m = sampler slope  
b = sampler intercept  
Ta = actual temperature (deg K)  
Pa = actual pressure (mm Hg)  
Ts = Average temperature (deg K)  
Ps = Average pressure (mm Hg)

Average I(chart): 49.2  
Average Flow over Sample (m3/min)  
0.943968028  
Enter Total Time (Hrs): 24.0  
Total flow over sample (m3/min)  
1359.31396  
Total flow over sample (CFM)  
47997.37592

NOTE: Ensure calibration orifice has been certified within 12 months of use

Tisch Environmental 145 South Miami Ave, Cleves OH 45002 • 877.263.7610 • sales@tisch-env.com • www.tisch-env.com



## PM10 High Volume Sampler Verification

### Site Information

Location: - Site ID: - Date: 23 December 2024  
Sampler: TE-6070 PM10 Serial No: 1313 Tech: Tong P.

### Site Conditions

Barometric Pressure (in Hg): 28.20 Corrected Pressure (mm Hg): 716.3  
Temperature (deg F): 76.1 Temperature (deg K): 297.5  
Average Press. (in Hg): 27.30 Corrected Average (mm Hg): 693.4  
Average Temp. (deg F): 75.3 Average Temp. (deg K): 297.1

### Calibration Orifice

Make: Tisch Environmental, Inc. Qstd Slope: 1.58407  
Model: TE-5028A Qstd Intercept: -0.01510  
Serial#: 1179 Calibration Due Date: 22 Oct 25

### Calibration Data

Plate or Test #	In H2O	Qa (m3/min)	I (chart)	IC (corrected)	Linear Regression
1	8.70	1.210	60.2	38.80	Slope 34.7912
2	7.20	1.101	55.3	35.64	Intercept -3.1851
3	6.10	1.014	49.9	32.16	Corr. Coeff 0.9950
4	5.30	0.946	44.8	28.87	SFR 1.096
5	3.80	0.803	39.0	25.13	SSP 54.20
# of Observations:					5

### Calculations

$Qa = 1/m(\sqrt{(H2O)(Ta/Pa)})-b$   
 $IC = I(\sqrt{(Ta/Pa)})$

$SFR = 1.13(Ps/Pa)(Ta/Ts)$   
 $SSP = (m*SFR+b)(\sqrt{(Pa/Ta)})$


m = sampler slope  
b = sampler intercept  
I = chart response  
Tav = daily average temperature  
Pav = daily average pressure

Qa = actual flow rate  
IC = corrected chart response  
m = calibrator slope  
b = calibrator intercept  
Ta = actual temperature (deg K)  
Pa = actual pressure (mm Hg)  
For subsequent calculation of sampler flow:

SFR = sampler set point flow rate  
SSP = sampler chart set point  
m = sampler slope  
b = sampler intercept  
Ta = actual temperature (deg K)  
Pa = actual pressure (mm Hg)  
Ts = Average temperature (deg K)  
Ps = Average pressure (mm Hg)

NOTE: Ensure calibration orifice has been certified within 12 months of use

Average I(chart): 49.8  
Average Flow over Sample (m3/min)  
1.029172473  
Enter Total Time (Hrs): 24.0  
Total flow over sample (m3/min)  
1482.008362  
Total flow over sample (CFM)  
52329.71525



## PM10 High Volume Sampler Verification

### Site Information

Location: - Site ID: - Date: 20 September 2024  
Sampler: TE-6070 PM10 Serial No: 3183 Tech: Tong P.

### Site Conditions

Barometric Pressure (in Hg): 27.03 Corrected Pressure (mm Hg): 686.6  
Temperature (deg F): 75.4 Temperature (deg K): 297.1  
Average Press. (in Hg): 26.73 Corrected Average (mm Hg): 678.9  
Average Temp. (deg F): 75.9 Average Temp. (deg K): 297.4

### Calibration Orifice

Make: Tisch Environmental, Inc. Qstd Slope: 1.57894  
Model: TE-5028A Qstd Intercept: -0.01520  
Serial#: 1179 Calibration Due Date: 10 Dec 24

### Calibration Data

Plate or Test #	In H2O	Qa (m3/min)	I (chart)	IC (corrected)	Linear Regression
1	9.40	1.287	60.0	39.47	Slope 30.7100
2	7.80	1.173	57.3	37.69	Intercept 0.7813
3	6.50	1.072	52.9	34.80	Corr. Coeff 0.9489
4	5.80	1.037	50.3	33.09	SFR 1.116
5	5.05	1.006	45.7	30.06	SSP 53.31
# of Observations:					5

### Calculations

$Qa = 1/m(\sqrt{(H2O)(Ta/Pa)})-b$   
 $IC = I(\sqrt{(Ta/Pa)})$

$SFR = 1.13(Ps/Pa)(Ta/Ts)$   
 $SSP = (m*SFR+b)(\sqrt{(Pa/Ta)})$


m = sampler slope  
b = sampler intercept  
I = chart response  
Tav = daily average temperature  
Pav = daily average pressure

Qa = actual flow rate  
IC = corrected chart response  
m = calibrator slope  
b = calibrator intercept  
Ta = actual temperature (deg K)  
Pa = actual pressure (mm Hg)  
For subsequent calculation of sampler flow:

SFR = sampler set point flow rate  
SSP = sampler chart set point  
m = sampler slope  
b = sampler intercept  
Ta = actual temperature (deg K)  
Pa = actual pressure (mm Hg)  
Ts = Average temperature (deg K)  
Ps = Average pressure (mm Hg)

NOTE: Ensure calibration orifice has been certified within 12 months of use

Average I(chart): 53.2  
Average Flow over Sample (m3/min)  
1.121929464  
Enter Total Time (Hrs): 24.0  
Total flow over sample (m3/min)  
1615.578428  
Total flow over sample (CFM)  
57046.0743



Trade & Engineering

## PM10 High Volume Sampler Verification

### Site Information

Location: - Site ID: - Date: 27 September 2024  
Sampler: TE-6070 PM10 Serial No: 3286 Tech: Tong P.

### Site Conditions

Barometric Pressure (in Hg): 27.30 Corrected Pressure (mm Hg): 693.4  
Temperature (deg F): 76.2 Temperature (deg K): 297.6  
Average Press. (in Hg): 26.70 Corrected Average (mm Hg): 678.2  
Average Temp. (deg F): 76.3 Average Temp. (deg K): 297.6

### Calibration Orifice

Make: Tisch Environmental, Inc. Qstd Slope: 1.57894  
Model: TE-5028A Qstd Intercept: -0.01520  
Serial#: 1179 Calibration Due Date: 10 Dec 24

### Calibration Data

Plate or Test #	In H2O	Qa (m3/min)	I (chart)	IC (corrected)	Linear Regression
1	9.50	1.288	62.1	40.68	Slope 34.2249
2	7.55	1.150	56.1	36.75	Intercept -3.0352
3	6.45	1.063	51.9	34.00	Corr. Coeff 0.9864
4	5.30	1.037	49.9	32.69	SFR 1.105
5	5.05	1.006	46.5	30.46	SSP 53.10

# of Observations: 5

### Calculations

$Qa = 1/m(\text{Sqrt}((H2O)(Ta/Pa))-b)$   
 $IC = I(\text{Sqrt}(Ta/Pa))$

$SFR = 1.13(Ps/Pa)(Ta/Ts)$   
 $SSP = (m*SFR+b)(\text{Sqrt}(Pa/Ta))$

Qa = actual flow rate  
IC = corrected chart response  
m = calibrator slope

SFR = sampler set point flow rate  
SSP = sampler chart set point  
m = sampler slope

b = calibrator intercept  
Ta = actual temperature (deg K)  
Pa = actual pressure (mm Hg)  
For subsequent calculation of sampler flow:

b = sampler intercept  
Ta = actual temperature (deg K)  
Pa = actual pressure (mm Hg)  
Ts = Average temperature (deg K)  
Ps = Average pressure (mm Hg)

m = sampler slope  
b = sampler intercept  
I = chart response  
Tav = daily average temperature  
Pav = daily average pressure

Average I(chart): 53.3  
Average Flow over Sample (m3/min)  
1.120345001  
Enter Total Time (Hrs) 24.0  
Total flow over sample (m3/min)  
1613.296801  
Total flow over sample (CFM)  
56965.51004

NOTE: Ensure calibration orifice has been certified within 12 months of use

เอกสารการสอบเทียบเครื่องมือตรวจวัดความสิ้นสะเทือน



ELECTRICAL AND ELECTRONICS INSTITUTE  
FOUNDATION FOR INDUSTRIAL DEVELOPMENT

975 Moo 4, Bangpoo Industrial Estate, Soi 8, Sukhumvit Road km 37

Phraek Sa, Mueang Samut Prakan, Samut Prakan 10280

Tel: +66 2709 4860 Fax: +66 2324 0917

Certificate No.: CP20250099EA  
Operation No.: CP2025030090

Certificate of Calibration

Equipment: Vibration Meter  
Manufacturer: InstanTel  
Model/Type: Micromate  
Serial No.: UM15904  
ID No.: VB-01-002  
Customer: C.E.M. Technology (Thailand) Co.,Ltd.  
Address: 31/8 Moo 13 T.Rai Khung, A.Sam Phran,  
Nakorn Phatom 73210  
Received Date: 7 March 2025  
Calibrated Date: 14 - 18 March 2025  
Issued Date: 19 March 2025  
Calibrated by: Ms. Juntaporn Kunhakom

Approved by:   
( Mr. Sittichai Swaksuriyawong )  
Group Manager

This report was prepared electronically using applicable electronic signature. Printing or copy of file are considered as a copy of the document.

The reported uncertainty of measurement was based on standard uncertainty multiplied by a coverage factor (k) providing a level of confidence of approximately 95%. This certificate may not be reproduced other than in full except with the prior written approval of the Electrical and Electronics Institute, Foundation for Industrial Development.



ELECTRICAL AND ELECTRONICS INSTITUTE  
FOUNDATION FOR INDUSTRIAL DEVELOPMENT

Certificate No.: CP20250099EA

Calibration Report

Equipment: Vibration Meter  
Manufacturer: InstanTel  
Model: Micromate  
Serial No.: UM15904  
ID No.: VB-01-002  
Ambient Temperature: ( 23 ± 5 ) °C  
Relative Humidity: ( 50 ± 15 ) %

Method of Calibration :-

In-house method : CC-SV004 by comparison with standard accelerometer.

Condition of this result of calibration

1. Reference standards instrument :-

Instrument	Model	Serial No.	Cert. No.	Due Date
1) Standard Accelerometer	8305	2708237	AV-0040-24	19-Sep-2025
2) Measuring Amplifier	2525	2685967	AV-0034-24	7-Aug-2025
3) LAN XI Analyzer	3160-4-042	3060-106135	CQ20240016EA	1-Dec-2025
4) Humidity and Temperature Transmitter	HMT331	K3810009	CD20240141EA	12-Jun-2025

2. This result of calibration was found accurate as shown on date and place of calibration only.

3. This certification is traceable to the international system of unit maintained at :-

- National Institute of Metrology (Thailand)
- Electrical and Electronics Institute; NSC Accredited Calibration No.0119





ELECTRICAL AND ELECTRONICS INSTITUTE  
FOUNDATION FOR INDUSTRIAL DEVELOPMENT

Certificate No.: CP20250099EA

Calibration Report

Result of Calibration:-

Function : Frequency response and Linearity test at 16 Hz

Frequency (Hz)	Nominal (mm/s)	Standard (mm/s)	UUC (mm/s)	Deviation (mm/s)	Uncertainty $\pm$ (%)	Direction
4.0	10.000	10.001	10.357	0.356	1.50	Longitudinal (L)
5.0	10.000	9.998	10.246	0.248	1.50	
6.3	10.000	10.000	10.372	0.372	1.50	
8.0	10.000	9.998	10.144	0.146	1.50	
10.0	10.000	10.008	10.089	0.081	1.50	
12.5	10.000	10.008	9.955	-0.053	1.60	
16.0	10.000	9.996	10.057	0.061	1.60	
	20.000	19.997	19.943	-0.054	1.60	
	30.000	29.970	29.864	-0.105	1.50	
	50.000	49.992	49.695	-0.297	1.50	
20.0	10.000	9.993	10.057	0.064	1.60	
25.0	10.000	9.998	10.077	0.079	1.50	
31.5	10.000	9.996	10.073	0.077	1.50	
40.0	10.000	9.996	10.120	0.124	1.50	
52.0	10.000	10.008	10.238	0.230	1.50	
63.0	10.000	9.991	10.388	0.397	1.50	
80.0	10.000	9.994	10.593	0.599	1.50	



ELECTRICAL AND ELECTRONICS INSTITUTE  
FOUNDATION FOR INDUSTRIAL DEVELOPMENT

Certificate No.: CP20250099EA

Calibration Report

Function : Frequency response and Linearity test at 16 Hz (Cont.)

Frequency (Hz)	Nominal (mm/s)	Standard (mm/s)	UUC (mm/s)	Deviation (mm/s)	Uncertainty $\pm$ (%)	Direction
4.0	10.000	10.003	10.104	0.101	1.50	Transverse (T)
5.0	10.000	9.996	10.069	0.073	1.60	
6.3	10.000	10.006	10.136	0.130	1.60	
8.0	10.000	10.011	9.957	-0.054	1.60	
10.0	10.000	10.008	9.953	-0.055	1.60	
12.5	10.000	9.998	9.939	-0.059	1.60	
16.0	10.000	10.000	9.915	-0.085	1.50	
	20.000	19.997	19.807	-0.190	1.50	
	30.000	29.995	29.738	-0.257	1.50	
	50.000	49.992	49.553	-0.439	1.50	
20.0	10.000	10.010	9.955	-0.055	1.60	
25.0	10.000	10.006	9.947	-0.059	1.60	
31.5	10.000	9.993	10.045	0.052	1.70	
40.0	10.000	10.003	10.059	0.056	1.50	
52.0	10.000	10.006	10.152	0.146	1.50	
63.0	10.000	10.001	10.309	0.308	1.50	
80.0	10.000	9.998	10.472	0.474	1.50	



ELECTRICAL AND ELECTRONICS INSTITUTE  
FOUNDATION FOR INDUSTRIAL DEVELOPMENT

Certificate No.: CP20250099EA

Calibration Report

Function : Frequency response and Linearity test at 16 Hz (Cont.)

Frequency (Hz)	Nominal (mm/s)	Standard (mm/s)	UUC (mm/s)	Deviation (mm/s)	Uncertainty ± (%)	Direction
4.0	10.000	10.006	9.663	-0.343	1.50	Vertical (V)
5.0	10.000	9.997	9.632	-0.365	1.50	
6.3	10.000	9.998	9.813	-0.185	1.50	
8.0	10.000	10.010	9.766	-0.244	1.50	
10.0	10.000	9.996	9.851	-0.145	1.60	
12.5	10.000	10.000	9.923	-0.077	1.50	
16.0	10.000	9.997	10.059	0.062	1.60	
	20.000	19.997	20.050	0.063	1.60	
	30.000	29.995	30.051	0.066	1.60	
	50.000	49.992	50.215	0.223	1.50	
20.0	10.000	10.004	10.175	0.171	1.50	
25.0	10.000	10.001	10.183	0.182	1.50	
31.5	10.000	10.008	10.175	0.167	1.50	
40.0	10.000	9.997	10.294	0.297	1.50	
52.0	10.000	9.998	10.617	0.619	1.50	
63.0	10.000	10.013	10.672	0.659	1.50	
80.0	10.000	10.006	10.940	0.934	1.50	

Remark 1. UUC: Unit Under Calibration  
2. The coverage factor  $k = 2.00$

-- End of Report --



ELECTRICAL AND ELECTRONICS INSTITUTE  
FOUNDATION FOR INDUSTRIAL DEVELOPMENT

975 Moo 4, Bangpoo Industrial Estate, Soi 8, Sukhumvit Road km 37

Phraek Sa, Mueang Samut Prakan, Samut Prakan 10280

Tel: +66 2709 4860 Fax: +66 2324 0917

Certificate No.: CP20250114EA

Operation No.: CP2025030100

Certificate of Calibration

Equipment: Vibration Meter

Manufacturer: InstanTel

Model/Type: Micromate

Serial No.: UM16048

ID No.: VB-01-003

Customer: C.E.M. Technology (Thailand) Co.,Ltd.

Address: 31/8 Moo 13 T.Rai Khung, A.Sam Phran,  
Nakorn Phatom 73210

Received Date: 18 March 2025

Calibrated Date: 9 - 10 April 2025

Issued Date: 11 April 2025

Calibrated by: Ms. Juntaporn Kunhakom

Approved by: \_\_\_\_\_

( Mr. Sittichai Swaksuriyawong )  
Group Manager

This report was prepared electronically using applicable electronic signature. Printing or copy of file are considered as a copy of the document.

The reported uncertainty of measurement was based on standard uncertainty multiplied by a coverage factor ( $k$ ) providing a level of confidence of approximately 95%. This certificate may not be reproduced other than in full except with the prior written approval of the Electrical and Electronics Institute, Foundation for Industrial Development.



ELECTRICAL AND ELECTRONICS INSTITUTE  
FOUNDATION FOR INDUSTRIAL DEVELOPMENT

Certificate No.: CP20250114EA

Calibration Report

Equipment: Vibration Meter  
Manufacturer: InstanTel  
Model: Micromate  
Serial No.: UM16048  
ID No.: VB-01-003  
Ambient Temperature: ( 23 ± 5 ) °C  
Relative Humidity: ( 50 ± 15 ) %

Method of Calibration :-

In-house method : CC-SV004 by comparison with standard accelerometer.

Condition of this result of calibration

1. Reference standards instrument :-

	Instrument	Model	Serial No.	Cert. No.	Due Date
1)	Standard Accelerometer	8305	2708237	AV-0040-24	19-Sep-2025
2)	Measuring Amplifier	2525	2685967	AV-0034-24	7-Aug-2025
3)	LAN XL Analyzer	3160-4-042	3060-106135	CQ20240016EA	1-Dec-2025
4)	Humidity and Temperature Transmitter	HMT331	K3810009	CD20240141EA	12-Jun-2025

2. This result of calibration was found accurate as shown on date and place of calibration only.

3. This certification is traceable to the international system of unit maintained at :-

- National Institute of Metrology (Thailand)
- Electrical and Electronics Institute; NSC Accredited Calibration No.0119



ELECTRICAL AND ELECTRONICS INSTITUTE  
FOUNDATION FOR INDUSTRIAL DEVELOPMENT

Certificate No.: CP20250114EA

Calibration Report

Result of Calibration:-

Function : Frequency response and Linearity test at 16 Hz

Frequency (Hz)	Nominal (mm/s)	Standard (mm/s)	UUC (mm/s)	Deviation (mm/s)	Uncertainty ± (%)	Direction
4.0	10.000	10.001	9.860	-0.141	1.50	Longitudinal (L)
5.0	10.000	9.998	9.886	-0.112	1.50	
6.3	10.000	9.994	10.059	0.065	1.60	
8.0	10.000	10.006	9.915	-0.091	1.50	
10.0	10.000	10.008	9.923	-0.085	1.50	
12.5	10.000	10.006	9.900	-0.106	1.50	
15.0	10.000	10.001	9.923	-0.078	1.50	
	20.000	19.997	19.878	-0.119	1.50	
	30.000	29.970	29.754	-0.216	1.50	
	50.000	49.992	49.567	-0.426	1.50	
20.0	10.000	10.010	9.956	-0.054	1.60	
25.0	10.000	9.996	10.046	0.050	1.60	
31.5	10.000	9.998	10.049	0.051	1.60	
40.0	10.000	10.006	10.089	0.083	1.50	
50.0	10.000	10.008	10.128	0.120	1.50	
63.0	10.000	9.991	10.262	0.271	1.50	
80.0	10.000	9.994	10.428	0.434	1.50	



ELECTRICAL AND ELECTRONICS INSTITUTE  
FOUNDATION FOR INDUSTRIAL DEVELOPMENT

Certificate No.: CP20250114EA

Calibration Report

Function : Frequency response and Linearity test at 16 Hz (Cont.)

Frequency (Hz)	Nominal (mm/s)	Standard (mm/s)	UUC (mm/s)	Deviation (mm/s)	Uncertainty ± (%)	Direction
4.0	10.000	9.997	10.104	0.107	1.50	Transverse (T)
5.0	10.000	9.996	10.089	0.093	1.50	
6.3	10.000	10.013	10.302	0.289	1.50	
8.0	10.000	9.998	10.081	0.083	1.60	
10.0	10.000	9.998	10.089	0.091	1.60	
12.5	10.000	10.003	10.081	0.078	1.60	
16.0	10.000	9.996	10.059	0.063	1.60	
	20.000	19.983	20.041	0.058	1.60	
	30.000	29.995	29.939	-0.056	1.60	
	50.000	49.992	49.868	-0.124	1.50	
20.0	10.000	9.998	10.097	0.099	1.50	
25.0	10.000	10.006	10.112	0.106	1.50	
31.5	10.000	9.998	10.128	0.130	1.50	
40.0	10.000	10.003	10.207	0.204	1.50	
52.0	10.000	10.006	10.278	0.272	1.50	
63.0	10.000	10.001	10.467	0.466	1.50	
80.0	10.000	9.998	10.648	0.650	1.50	



ELECTRICAL AND ELECTRONICS INSTITUTE  
FOUNDATION FOR INDUSTRIAL DEVELOPMENT

Certificate No.: CP20250114EA

Calibration Report

Function : Frequency response and Linearity test at 16 Hz (Cont.)

Frequency (Hz)	Nominal (mm/s)	Standard (mm/s)	UUC (mm/s)	Deviation (mm/s)	Uncertainty ± (%)	Direction
4.0	10.000	10.006	10.104	0.098	1.50	Vertical (V)
5.0	10.000	9.990	10.057	0.067	1.60	
6.3	10.000	9.998	10.262	0.264	1.50	
8.0	10.000	10.010	10.112	0.102	1.50	
10.0	10.000	9.998	10.144	0.146	1.50	
12.5	10.000	10.000	10.168	0.168	1.50	
16.0	10.000	9.994	10.191	0.197	1.50	
	20.000	19.997	20.288	0.291	1.50	
	30.000	29.995	30.290	0.295	1.50	
	50.000	49.992	50.459	0.467	1.50	
20.0	10.000	10.003	10.278	0.275	1.50	
25.0	10.000	10.001	10.570	0.569	1.50	
31.5	10.000	9.994	10.144	0.150	1.50	
40.0	10.000	10.006	10.286	0.280	1.50	
52.0	10.000	9.994	10.491	0.497	1.50	
63.0	10.000	10.013	10.585	0.572	1.50	
80.0	10.000	10.006	10.790	0.784	1.50	

Remark 1. UUC: Unit; Under Calibration  
2. The coverage factor  $k = 2.00$

-- End of Report --





ELECTRICAL AND ELECTRONICS INSTITUTE  
FOUNDATION FOR INDUSTRIAL DEVELOPMENT

975 Moo 4, Bangpoo Industrial Estate, Soi 8, Sukhumvit Road km 37

Phraek Sa, Mueang Samut Prakan, Samut Prakan 10280

Tel: +66 2709 4860 Fax: +66 2324 0917

Certificate No.: CP20240325EA  
Operation No.: CP2024080270

## Certificate of Calibration

Equipment: Vibration Meter  
Manufacturer: Instantel  
Model/Type: Micromate  
Serial No.: UM20454  
ID No.: VB-01-008  
Customer: C.E.M. Technology (Thailand) Co.,Ltd.  
Address: 31/8 Moo 13 T.Rai Khung, A.Sam Phran,  
Nakorn Phatom 73210  
Received Date: 2 August 2024  
Calibrated Date: 28 - 29 August 2024  
Issued Date: 2 September 2024  
Calibrated by: Ms. Juntaporn Kunhakom

Approved by:   
( Mr. Sittichai Swaksuriyawong )  
Group Manager

This report was prepared electronically using applicable electronic signature. Printing or copy of file are considered as a copy of the document.

The reported uncertainty of measurement was based on standard uncertainty multiplied by a coverage factor (k) providing a level of confidence of approximately 95%. This certificate may not be reproduced other than in full except with the prior written approval of the Electrical and Electronics Institute, Foundation for Industrial Development.



ELECTRICAL AND ELECTRONICS INSTITUTE  
FOUNDATION FOR INDUSTRIAL DEVELOPMENT

Certificate No.: CP20240325EA

## Calibration Report

Equipment: Vibration Meter  
Manufacturer: Instantel  
Model: Micromate  
Serial No.: UM20454  
ID No.: VB-01-008  
Ambient Temperature: ( 23 ± 5 ) °C  
Relative Humidity: ( 50 ± 15 ) %

### Method of Calibration :-

In-house method : CC-SV004 by comparison with standard accelerometer.

### Condition of this result of calibration

1. Reference standards instrument :-

Instrument	Model	Serial No.	Cert. No.	Due Date
1) Standard Accelerometer	8305-001	30120	AV-0028-24	23-Jun-2025
2) Measuring Amplifier	2525	3016651	AV-0029-24	23-Jun-2025
3) PULSE Multi-analyzer system	3050-A-060	3050-110127	CQ20230024EA	5-Nov-2024
4) PULSE Multi-analyzer system	3160-4-042	3060-106135	CQ20230025EA	5-Nov-2024
5) Humidity and Temperature Transmitter	HMT331	K3810009	CD20240141EA	12-Jun-2025

2. This result of calibration was found accurate as shown on date and place of calibration only.

3. This certification is traceable to the international system of unit maintained at :-  
- National Institute of Metrology (Thailand)

Certificate No.: CP20240325EA

### Calibration Report

#### Result of Calibration:-

Function : Frequency response and Linearity test at 16 Hz

Frequency (Hz)	Nominal (mm/s)	Standard (mm/s)	UUC (mm/s)	Deviation (mm/s)	Uncertainty $\pm$ (%)	Direction
4.0	10.000	10.006	10.546	0.540	1.50	Longitudinal (L)
5.0	10.000	9.998	10.585	0.587	1.50	
6.3	10.000	9.998	10.806	0.808	1.50	
8.0	10.000	10.008	10.499	0.491	1.50	
10.0	10.000	9.998	10.483	0.485	1.50	
12.5	10.000	10.020	10.467	0.447	1.50	
16.0	10.000	10.004	10.309	0.305	1.50	
	20.000	19.997	20.706	0.709	1.50	
	30.000	30.010	31.031	1.021	1.50	
	50.000	49.992	51.484	1.492	1.50	
20.0	10.000	10.003	10.428	0.425	1.50	
25.0	10.000	10.007	10.420	0.413	1.50	
31.5	10.000	10.013	10.380	0.367	1.50	
40.0	10.000	10.001	10.341	0.340	1.50	
50.0	10.000	10.013	10.428	0.415	1.50	
52.0	10.000	10.001	10.502	0.501	1.50	
63.0	10.000	9.991	10.546	0.555	1.50	
80.0	10.000	9.998	10.522	0.524	1.50	

Certificate No.: CP20240325EA

### Calibration Report

Function : Frequency response and Linearity test at 16 Hz (Cont.)

Frequency (Hz)	Nominal (mm/s)	Standard (mm/s)	UUC (mm/s)	Deviation (mm/s)	Uncertainty $\pm$ (%)	Direction
4.0	10.000	10.003	10.428	0.425	1.50	Transverse (T)
5.0	10.000	10.001	10.483	0.482	1.50	
6.3	10.000	10.020	10.885	0.865	1.50	
8.0	10.000	9.987	10.530	0.543	1.50	
10.0	10.000	9.997	10.609	0.612	1.50	
12.5	10.000	10.000	10.530	0.530	1.50	
16.0	10.000	10.001	10.372	0.371	1.50	
	20.000	19.997	20.769	0.772	1.50	
	30.000	29.995	31.133	1.138	1.50	
	50.000	49.992	51.721	1.729	1.50	
20.0	10.000	10.003	10.420	0.417	1.50	
25.0	10.000	10.013	10.380	0.367	1.50	
31.5	10.000	9.994	10.309	0.315	1.50	
40.0	10.000	10.003	10.254	0.251	1.50	
50.0	10.000	10.006	10.349	0.343	1.50	
52.0	10.000	9.996	10.412	0.416	1.50	
63.0	10.000	10.006	10.467	0.461	1.50	
80.0	10.000	9.987	10.459	0.472	1.50	

Certificate No.: CP20240325EA

### Calibration Report

Function : Frequency response and Linearity test at 16 Hz (Cont.)

Frequency (Hz)	Nominal (mm/s)	Standard (mm/s)	UUC (mm/s)	Deviation (mm/s)	Uncertainty ± (%)	Direction
4.0	10.000	10.008	9.742	-0.266	1.50	Vertical (V)
5.0	10.000	10.020	9.710	-0.310	1.50	
6.3	10.000	10.008	9.931	-0.077	1.50	
8.0	10.000	10.003	9.632	-0.371	1.50	
10.0	10.000	10.000	9.703	-0.297	1.50	
12.5	10.000	10.001	9.710	-0.291	1.50	
16.0	10.000	10.003	9.758	-0.245	1.50	
	20.000	19.997	19.705	-0.292	1.50	
	30.000	29.995	29.549	-0.446	1.50	
	50.000	49.978	49.127	-0.851	1.50	
20.0	10.000	10.008	9.860	-0.148	1.50	
25.0	10.000	9.997	9.513	-0.484	1.50	
31.5	10.000	9.995	9.915	-0.080	1.50	
40.0	10.000	9.993	10.041	0.048	1.50	
50.0	10.000	9.993	10.207	0.214	1.50	
52.0	10.000	9.984	10.246	0.262	1.50	
63.0	10.000	9.983	10.404	0.421	1.50	
80.0	10.000	10.025	10.720	0.695	1.50	

Remark 1. UUC: Unit Under Calibration  
2. The coverage factor  $k = 2.00$

-- End of Report --


เอกสารการสอบเทียบเครื่องมือตรวจวัดคุณภาพน้ำ

# CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhaprachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech.cal@yahoo.com, calibratech.cal@hotmail.com



## Certificate of Calibration

**Certificate No. :** 68-400172-1

**Page : 1 of 2**

**Submitted by :** C.E.M Technology (Thailand) Co., Ltd.  
219/43 Moo.12 Petchkasem Rd, Omnoi, Krathumban, Samutsakom 74130 (Head Office)

**Equipment :** Temperature controlled enclosure (Refrigerator)  
Manufacturer : Samchai Model : LD2 DC 70  
Range : N/A °C Resolution : 1 °C  
Serial No. : 85545 ID No. : N/A

**Environment :** On site calibration was carried out at the Laboratory,  
C.E.M Technology (Thailand) Co., Ltd.  
Ambient Temperature : (27.0 to 28.0) °C  
Relative Humidity : (50 to 55) %  
Line Voltage : (223.0 to 225.0) V

**Date of Received :** 21 March 2025

**Date of Calibration :** 21 March 2025

**Date of Issue :** 22 March 2025

**Calibrated by :** Permpoon Chanpu

**Calibration Method :** CAL-M4004, TLAS G-20

The temperature scale used was based on ITS-90

**Reference Standard Instruments :** This certification is traceable to the International System of Units  
Standard Digital Thermometer with RTD Probe

ID No.	Cert. No.	Due Date	Traceability
400046 & 400047	68-400007-2	29 Jul 2025	National Institute of Metrology Thailand (NIMT)

Approved by :   
( Permpoon Chanpu )  
Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



CAL-F0031-03

# CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhaprachasan 3 Rd. Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech.cal@yahoo.com, calibratech.cal@hotmail.com

## Certificate of Calibration

**Certificate No. : 68-400172-1**


**Page : 2 of 2**

**Result of Calibration :** Without Adjustment

**UUC Condition As-Received :** Good

**Function :** Temperature measurement

This instrument was setting air ventilation at position 0 (close)

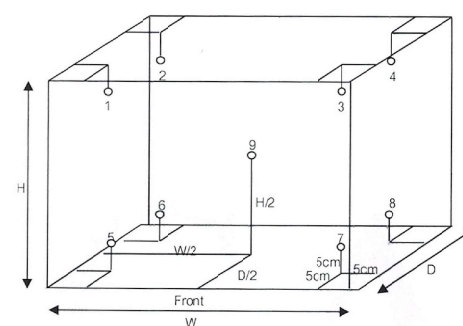

Inside of Chamber  
W = 1.13 m  
D = 0.51 m  
H = 1.34 m  
Capacity = 0.77 m<sup>3</sup>

Test Point ( °C )	Setting Temperature ( °C )	Indicating Temperature ( °C )	Measured Temperature ( °C ) @ Sensor No.									Uncertainty ( ± °C )
			1	2	3	4	5	6	7	8	9	
4	4	4	5.13	4.85	3.25	3.11	4.43	4.77	2.75	2.77	4.01	0.73

Test Point ( °C )	Setting Temperature ( °C )	Indicating Temperature ( °C )	Measured Uniformity ( °C )	Measured Stability ( °C )	Overall Variation ( °C )
4	4	4	1.29	0.08	2.55

**Remark** The uncertainty is not combine uniformity of the air chamber

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k = 2 ,  
providing a level of confidence of approximately 95%

- oOo -



CAL-F0031-03



# CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhprachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech.cal@yahoo.com, calibratech.cal@hotmail.com



## Certificate of Calibration

Certificate No. : 68-400089-2

Page : 1 of 2

Submitted by : C.E.M Technology (Thailand) Co., Ltd.  
219/43 Moo.12 Petchkasem Rd, Omnoi, Krathumban, Samutsakorn 74130 (Head Office)

Equipment : Temperature Indicator with Thermistor Probe  
Temperature Indicator  
Manufacturer : XS Instruments Model : PC 5  
Range : N/A °C Resolution : 0.1 °C  
Serial No. : GB 0706/024 ID No. : WW-23-001  
Thermistor probe  
Model : N/A Sheath Material : Plastic  
Diameter : 10 mm. Length : 65 mm.  
Serial No. : GB 0706/024 ID No. : WW-23-001

Environment : On site calibration was carried out at the Laboratory,  
C.E.M Technology (Thailand) Co., Ltd.  
Ambient Temperature : (26.0 to 27.0) °C  
Relative Humidity : (45 to 50) %  
Line Voltage : (224.5 to 226.0) VAC

Date of Received : 11 February 2025

Date of Calibration : 11 February 2025

Date of Issue : 17 February 2025

Calibrated by : Permpon Chanpu

Calibration Method : This instrument was calibrated by In-house method comparison technique CAL-M4003  
by compared with PRT in the liquid bath at the constant controlled temperature.

The temperature scale used was based on ITS-90

Reference Standard Instruments : This certification is traceable to the International System: of Units

1. Platinum Resistance Thermometer (PRT)

ID No.	Cert. No.	Due Date	Traceability
400002	TT-0095-24	01 Jul 2026	National Institute of Metrology Thailand (NIMT)

2. Standard Digital Thermometer

ID No.	Cert. No.	Due Date	Traceability
400033	24E633	21 Feb 2026	National Institute of Metrology Thailand (NIMT)

Approved by :

( Permpon Chanpu )

Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



CAL-F0031-03

# CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhprachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech.cal@yahoo.com, calibratech.cal@hotmail.com

## Certificate of Calibration

Certificate No. : 68-400089-2

Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Function : Temperature measurement

Immersion Depth ( mm. )	Standard Reading ( °C )	UUC Reading ( °C )	Correction ( °C )	Uncertainty ( ± °C )
65	15.002	15.1	-0.1	0.19
65	30.005	30.0	0.0	0.19
65	45.004	44.9	0.1	0.19

Remark

UUC : Unit Under Calibration

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor  $k = 2$ ,  
providing a level of confidence of approximately 95%

- 000 -



CAL-F0031-03

# CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhprachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech.cal@yahoo.com, calibratech.cal@hotmail.com



NSC-TISI-TIS 17025  
CALIBRATION 0330

## Certificate of Calibration

Certificate No. : 68-430004-1

Page : 1 of 2

Submitted by :

C.E.M Technology (Thailand) Co.,Ltd.

219/43 Moo.12 Petchkasem Rd. Omnoi, Krathumban, Samutsakorn 74130 (Head Office)

Equipment :

Digital Conductivity meter (Pocket)

Manufacturer : XS Instruments Model : PC 5

Serial No. : GB 0706/024 ID No. : WW-23-001

Environment :

On site calibration was carried out at the Laboratory,

C.E.M Technology (Thailand) Co., Ltd.

Ambient Temperature (26.0 to 27.0) °C

Relative Humidity (45 to 50) %

Date of Received :

11 February 2025

Date of Calibration :

11 February 2025

Date of Issue :

17 February 2025

Calibrated by :

Permpoon Chanpu

Calibration Method :

In-house method CAL-M4301 direct measurement by conductivity buffer solution

Reference Standard Instruments : This certification is traceable to the International System of Units

Standard Buffer Solution

Material	Lot No.	Exp. Date	Traceability
84 µS/cm	0300	01 June 2027	National Institute of Standards and Technology (NIST), U.S.A., S.R.M.
1413 µS/cm	970986	25 April 2025	CPA Chem Ltd. Accredited to ISO 17034 and ISO/IEC 17025
12.88 mS/cm	970987	25 April 2025	CPA Chem Ltd. Accredited to ISO 17034 and ISO/IEC 17025

Approved by :

  
(Permpoon Chanpu)  
Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.

CAL-F0031-03



# CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhprachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech.cal@yahoo.com, calibratech.cal@hotmail.com

## Certificate of Calibration

Certificate No. : 68-430004-1

Page : 2 of 2

Result of Calibration :

UUC Condition As-Received : Good

Function : Conductivity measurement

Before Adjustment

Standard Conductivity Solution	UUC Reading	Correction	Uncertainty ( ± )	Unit
84*	79.7	4.3	1.1	µS/cm
1413	1602	-189	9.0	µS/cm
12.88	12.81	0.07	0.082	mS/cm

After Adjustment : at 84, 1413 µS/cm 12.880 mS/cm

Standard Conductivity Solution	UUC Reading	Correction	Uncertainty ( ± )	Unit
84*	84.0	0.0	1.1	µS/cm
1413	1413	0	9.0	µS/cm
12.88	12.88	0.00	0.082	mS/cm

Remark

UUC : Unit Under Calibration

\* This parameter are out of accreditation's scope.

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor  $k = 2$ ,  
providing a level of confidence of approximately 95%

- 000 -





CAL-F0031-03

## การดูแลบำรุงรักษาเชิงป้องกัน

### Preventive Maintenance



บริษัท ดีเคเอสเอช เทคโนโลยี จำกัด

ฝ่ายบริการหลังการขาย

โทร 0 2 639 7000 E-mail: [service.tec.th@dksh.com](mailto:service.tec.th@dksh.com)

ฝ่ายขายและการตลาด

โทร 0 2 639 7000 E-Mail : [marketing.tec.th@dksh.com](mailto:marketing.tec.th@dksh.com)

Website : [www.dksh.co.th/technology/scientific-thailand](http://www.dksh.co.th/technology/scientific-thailand)

#### เงื่อนไขการให้บริการ Preventive Maintenance

บริษัทฯ จะส่งวิศวกรผู้ชำนาญ เพื่อให้บริการตามขอบข่ายของการบริการ เฉพาะ ในวันและเวลา ราชการ หากมีความประสงค์ที่จะรับบริการนอกเหนือจากวัน เวลา ราชการ (วันหยุดเสาร์ – อาทิตย์ หรือวันหยุด นักชดถุญ) บริษัทฯ จะคิดค่าบริการเพิ่มเติมตามอัตราที่กฎหมายแรงงานกำหนดไว้

#### ขอบข่ายการบริการ

- ตรวจสอบสภาพการทำงานต่าง ๆ ของเครื่องมือ
- ทดสอบประสิทธิภาพการทำงานของเครื่องมือ
- รายการผลการตรวจสอบเครื่องมือ

#### หมายเหตุ

- ราคานี้ไม่รวมถึงค่าบริการซ่อม หรือ เปลี่ยนอะไหล่ที่ชำรุดเสียหาย หรือหมดสภาพการใช้งาน
- ในกรณีที่ผู้รับบริการอยู่นอกเขตพื้นที่ให้บริการ บริษัทฯ จำเป็นต้องคิดค่าใช้จ่ายเพิ่มเติม ได้แก่ ค่าเดินทาง เป็นต้น
- บริษัทฯ ขอสงวนสิทธิ์ในการเปลี่ยนแปลงราคา โดยไม่แจ้งให้ทราบล่วงหน้า



### ช่องทางการติดต่อ

DKSH Technology Limited (บริษัท ดีเคเอสเอช เทคโนโลยี จำกัด)  
เลขที่ 2533 ถนนสุขุมวิท แขวงบางจาก เขตพระโขนง กรุงเทพฯ 10260  
เลขประจำตัวผู้เสียภาษี 010-555-001-4547 (สำนักงานใหญ่)



Call center 0 2 639 7000



DKSH Scientific



[www.dksh.com/scientific-thailand](http://www.dksh.com/scientific-thailand)



[marketing.tec.th@dksh.com](mailto:marketing.tec.th@dksh.com)



@dkshscientific

### Preventive Maintenance Contract

จำนวนในการทำสัญญาบริการ ...1...ครั้งต่อปี

ครั้งที่ 1, วันที่ 14/05/2025.....

### รายละเอียดผู้รับบริการ

หน่วยงาน	บริษัท ซี.อี.เอ็ม เทคโนโลยี (ไทยแลนด์) จำกัด		
ที่อยู่	219/43 หมู่ 12 ถนนเพชรเกษม ตำบลอ้อมน้อย อำเภอกะทู้ภูเก็ต จังหวัดสมุทรสาคร 74130		
โทรศัพท์	0869054664	แฟกซ์	-

### ผู้ติดต่อ

ชื่อ - นามสกุล	คุณศิริภาพร พิมพ์			
ตำแหน่ง	เจ้าหน้าที่ห้องปฏิบัติการ			
โทรศัพท์	0869054664	เบอร์ต่อ	-	แฟกซ์ -
E-mail	lab.cemtech1@gmail.com			

### รายละเอียดผู้ให้บริการ

บริษัท ดีเคเอสเอช เทคโนโลยี จำกัด (ฝ่ายบริการหลังการขาย) (สำนักงานใหญ่)			
เลขที่ 2533 ถนนสุขุมวิท แขวงบางจาก เขตพระโขนง กรุงเทพฯ 10260			
โทรศัพท์ 0 2 693 7000 Email: Jirayut.js@dksh.com			
เจ้าหน้าที่ประสานงาน : คุณจิรายุช สลอาด			
เจ้าหน้าที่ผู้ให้บริการ	นายจิรายุช สลอาด		
ตำแหน่ง	Specialist, Technical Service.		
โทรศัพท์	0938138736	แฟกซ์	-
E-mail	Jirayut.js@dksh.com		

ลงนามผู้รับบริการ		ลงนามผู้ให้บริการ	<i>Jirayut Salyard</i>
ตัวบรรจง	(.....)	ตัวบรรจง	(นาย จิรายุช สลอาด)
ตำแหน่ง		ตำแหน่ง	Specialist, Technical Service.
วันที่ / ประทับตราบริษัท		วันที่ / ประทับตราบริษัท	14/05/2025




JOB:WQ-00070598.....MODEL:VAP 200.....S/N: GER5200180181

# Operational Qualification (OQ)

ตรวจสอบสภาพเครื่อง


## FRONT

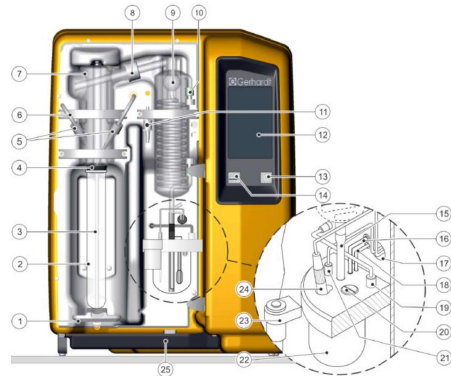

No		PASS	FAIL	N/A
1	Quick clamping device with clamping block	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
2	Digestion tube 250/300 ml	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
3	PTFE steam inlet tubing	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
4	Connection stopper , Viton	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
5	Screw cap GL18	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
6	PTFE-inlet tubing NaOH	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
7	Distribution head made of glass	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
8	Screw cap GL32	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
9	Distillation condenser made of glass	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
10	Screw cap GL14	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
11	Ventilation valve	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
12	Control panel	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
13	Operating Button	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
14	USB interface (with protective cap)	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
15	Silicone tubing 8/10 for distillate discharge **	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>
16	Verprene tubing 4/8 , receiver suction **	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>
17	Cable duct for electrode cable + titration tube**	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>
18	Silicone tubing 4/7 , boric acid inlet**	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>
19	Sensor for level monitoring including connector**	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>
20	Agitator motor with propeller**	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>
21	Titration acid inlet tube **	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>
22	Receiver glass**	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>
23	Holder for pH electrode , removable**	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>
24	pH electrode (combined electrode)**	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>
25	Drip tray PP	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>


\*\* only VAP 450

## REAR

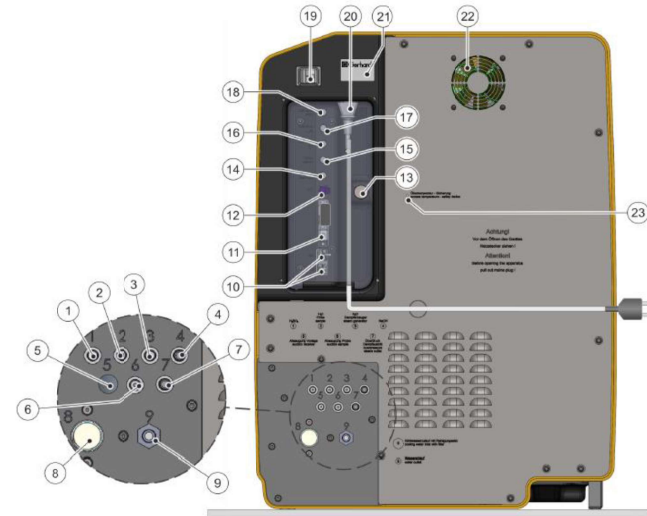


No		PASS	FAIL	N/A
1	Tube connection for sample H3BO3 supply	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>
2	Tube connection for sample H2O supply	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>
3	Tube connection for steam generator H2O supply	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
4	Tube connection for NaOH supply	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
5	Tube connection for receiver glass extraction	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
6	Tube connection for sample waste extraction	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
7	Tube connection , overpressure steam outlet	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
8	Connection for cooling water supply (with cleaning sieve)	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
9	Tube connection for cooling water outlet	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
10	4 X USB interface	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
11	1 X RS-232 Interface	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
12	LAN Interface	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
13	Screw cap for Perspex cover	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
14	Connection socket for sample waste tank level monitoring	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
15	Connection (not used)	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>
16	Connection socket for H2O tank level monitoring	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
17	Connection socket for H3BO3 tank level monitoring	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
18	Connection socket for NaOH tank level monitoring	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
19	Overcurrent circuit breaker	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
20	Apparatus socket (mains cable connection)	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
21	Rating plate with serial number	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
22	Exhaust air fan	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
23	Excess temperature switch	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>

## Inside Steam generator

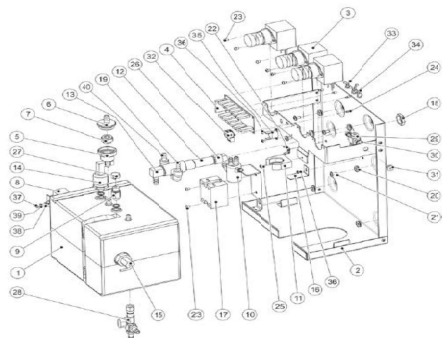

No		PASS	FAIL	N/A
1	Steam generator	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
2	Steam generator traverse	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
3	Pinch valve	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
4	Circuit board distributor	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
5	Valve tubing connection	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
6	Housing safety valve	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
7	Safety valve SKT	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
8	Excess temperature protection , steam generator	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
9	Safety valve G 1/8 0,5 bar	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
10	Ventilation glass pinch valve VAPODEST	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
11	Hose clamp for ventilation clamp	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
12	Distributor PP	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
13	Angle connection PP	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
14	Pressure transmitter	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
15	Level switch	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
16	Fixing bracket steam generator	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
17	Relay HT+	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
18	VA Hexagon nut 1/2"	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
19	Angle connection 1/8"	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
20	Bushing nipple 6-10-14	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
21	VA Lens head screw M5 X 10	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
22	Grounding connection , 2-pole	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
23	VA Lens head screw M4 X 6	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
24	Spacer bolt 5 mm	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
25	VA Lens head screw M4 X 10	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
26	Tubing connection	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
27	Hose clamp 14.5 mm	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
28	Module ball valve with nozzles	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
29	Cross manifold with spout	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
30	Seal copper G 1/8	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
31	Locking screw 1/8"	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
32	Pin strip	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
33	Bundle clamp 12 H 4500	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
34	Bundle clamp 12 H 4502	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
35	Temperature switch 80°C	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
36	VA Lens head screw M3 X 6	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
37	VA Hexagon nut M4	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
38	Lins head screw M4 X 8	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
39	VA Spring washer	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
40	Angle connection , reduced , 1/8" PP	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>

## Module Pump holder VAP200 - 450 V3

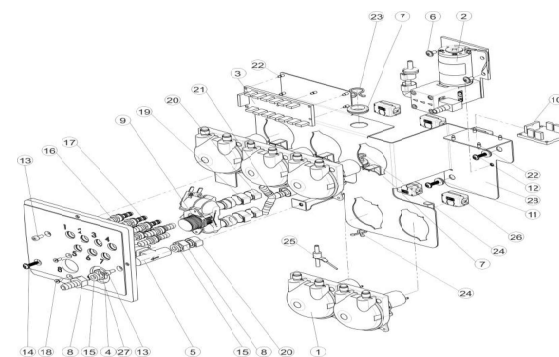

No		PASS	FAIL	N/A
1	Peristaltic pump	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
2	Diaphragm pump NaOH. with non-return valve	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
3	Circuit board	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
4	Tubing connection module	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
5	Flow controller	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
6	Lens head screw M5 x 10	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
7	Bushing nozzle	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
8	Screw in socket	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
9	Magnetic valve 2/2 way	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
10	Circuit board distributor	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
11	Bushing nozzle	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
12	Screw 5 x 25	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
13	Cylinder screw	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
14	Screw 5 x 20	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
15	Seal EPDM 15 x 4	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
16	Tubing connection piece 51x10x6,5	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
17	Tubing connection piece 51x10x10	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
18	Screw M4x10	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
19	Clamp	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
20	Clamp	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
21	Y-tube connector	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
22	Spacer bolt 5 mm	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
23	Bundle clamp	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
24	Bundle clamp	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
25	Retrofit earthing pumpv	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
26	Snap ferrite	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
27	Nut G 3/8"	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
28	Pump holder plate	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>

Control panel



No		PASS	FAIL
1	Title bar	<input checked="" type="checkbox"/>	<input type="checkbox"/>
2	Status bar	<input checked="" type="checkbox"/>	<input type="checkbox"/>
3	Navigation button	<input checked="" type="checkbox"/>	<input type="checkbox"/>
4	Smart switch with multiple functions	<input checked="" type="checkbox"/>	<input type="checkbox"/>
5	USB interface	<input checked="" type="checkbox"/>	<input type="checkbox"/>

รายละเอียดการตรวจสอบ

ขั้นตอนการบริการ

ตรวจสอบระบบไฟฟ้า (Electrical Test)

- ความต้านทานทางไฟฟ้าของเครื่องกับกราวด์
- กระแสไฟฟ้าที่ใช้งาน

ตรวจสอบสภาพเครื่อง (Optical Test)

- Main cable
- Electric wiring
- Pumps
- Distribution Head
- Condensor
- Steam generator
- Tubing
- Viton cone

ตรวจสอบ Function การทำงาน (The FunctionTest)

- ระบบสร้างและควบคุมความดันของ Steam
- ระบบการเติมน้ำเข้า Sample Tube
- ระบบการเติม Na OH
- ระบบการเติม H3BO3

## รายงานผลการให้บริการ

### 1. TECHNICAL DATA

Main Supply 220 volt + 10% 50 Hz with ground	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	Remark
Normal current	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	.....8a.....

### 1.1 COOLING WATER BATH

Temperature 15-20 °C	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	Remark
Cooling Water Outlet	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	
Control Temperature	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	

### 1.2 OPTICAL TEST VAP200

Screw cap GL14	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	Remark
Screw cap GL18	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	
Screw cap GL32	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	
Distillation Head	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	
Condensor	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	เปลี่ยน condensor ใหม่
Viton Cone	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	เปลี่ยน Viton cone
Ventilation Valve BV	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	
Micro Switch Sample	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	
Agitator motor for propeller	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	

### 2. SYSTEM COOLING WATER INLET

Cooling Water Inlet	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	Remark
Cooling Water Outlet	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	
Flow control valve	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	

### 3.SYSTEM CONTROL

Display	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	Remark
Program	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	
Adding NaOH	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	
Adding H2O	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	
Adding H3BO3	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	
Suction Sample	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	
Suction Receiver	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	

### 4.SYSTEM DISTILLATION

Boiler	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	Remark
Level Sensor	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	
Novopren	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	เปลี่ยน Novopren
Solenoid Valve Shut-Off	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	
Solenoid Valve Steam	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	
Solenoid Valve soft steam	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	
Ventilation Valve Premount	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	
Excess Pressure Detector	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	
Heating Element	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	

### 5. PUMP

	Pass	Fail	N/A	Remark
Pump H <sub>2</sub> O Steam	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	.....
- Non-Return Valve	-	-	-	.....
Pump H <sub>2</sub> O Sample	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	.....
- Non-Return Valve	-	-	-	.....
Pump NaOH	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	.....
- Non-Return Valve	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	.....
Pump H3BO3	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	.....
- Non-Return Valve	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	.....
Pump suction	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	.....
Pump suction receiver	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	.....

### 6. The Following Program Run :

	Pass	Fail	N/A	Remark
Addition H2O 0-999 ml.	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	.....
Addition NaOH 0-999 ml.	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	.....
Addition H3BO3 0-999 ml.	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	.....
Reaction Time 0-108 min	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	.....
Distillation Time 0-108 min	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	.....
Steam Capacity 10%-100%	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	.....
Suction Sample	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	.....
Suction Receiver	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	.....

### 7. Measured pumps

Pump NaOH	Volume : ..13.33.....ml	Remark
-----------	-------------------------	--------

Remark : .....เปลี่ยน condensor เปลี่ยนสกรูพ, viton cone เปลี่ยน novopren เปลี่ยน



ข้อมูลสนับสนุนด้านเทคนิค (General Technical Support)

การบำรุงรักษาทั่วไป ( Basic maintenance)

Cleaning program

Glass parts and tubes must be rinsed daily before starting analysis in order to prevent clogging by crystallising chemicals.  
The following settings are recommended for this:

parameters	Value
H <sub>2</sub> O addition	150 ml
NaOH addition	0 ml
Distillation time	7 min
Steam power	100 %
Reaction time	0 s
Suction sample	30 s

- Insert a digestion tube (without sample) and start the program.
- All liquid carrying parts are cleaned. In the case of strong soiling, approx. 10 ml of sulphuric acid can also be added to the digestion tube.

General error message

Fault description	Cause	Remedy
'Cooling water flow volume too low'	Cooling water pressure under 1 bar	<ul style="list-style-type: none"><li>Open water tap.</li><li>Check coolant pressure.</li><li>Check coolant tube.</li></ul> Program continues automatically once error has been fixed.
'Sample tube missing'	Sample tube missing.	<ul style="list-style-type: none"><li>Insert sample tube.</li></ul> Continue program or restart.
'Distillation room protective door open'	Protection door not closed	<ul style="list-style-type: none"><li>Close protection door.</li></ul> Program continues automatically once error has been fixed.
'Reagent storage/waste'	One or more storage tanks are empty	<ul style="list-style-type: none"><li>Fill storage tank.</li><li>Check correct sealing of the universal sensors.</li></ul> The running program can be continued after rectification of the error.
	The sample waste tank is full.	<ul style="list-style-type: none"><li>Empty sample waste tank.</li><li>Check correct sealing of the universal sensors.</li></ul> The running program can be continued after rectification of the error.

Analytical errors

Fault description	Cause	Remedy
Analysis results too high	The chemicals used are contaminated with nitrogen compounds.	<ul style="list-style-type: none"><li>Detailed checking of the chemicals.</li><li>Determination of a blank value.</li><li>Replace the chemicals if necessary.</li></ul>
	Violent reaction in the digestion tube, sodium hydroxide drops get into the receiver.	<ul style="list-style-type: none"><li>Increase of the water addition amount.</li></ul>
	Glass bridge of the condenser is broken or worn out, sodium hydroxide drops get into the receiver.	<ul style="list-style-type: none"><li>Replacement of the glass condenser.</li></ul>
	Glass cleaning agents in the digestion tube.	<ul style="list-style-type: none"><li>Clean digestion tube in advance with distilled water.</li></ul>
	Entrainment of ammonia from the previous sample.	<ul style="list-style-type: none"><li>Increase distillation time.</li><li>Check whether the sample was previously sufficiently alkalisied.</li></ul>
Analysis result too low or no result	Incomplete distillation; distillation time too short.	<ul style="list-style-type: none"><li>No quantitative expulsion of the ammonia content.</li><li>The distillation amount should be 100 ml.</li></ul>
	Ammonia escapes at leaking places.	<ul style="list-style-type: none"><li>Solled or defective Viton plugs; clean or replace.</li><li>Check seals (GL screw connections) on the distribution head; replace if necessary.</li><li>Check valve at the condenser is gummed up; clean or replace.</li><li>Digestion tube is damaged at the neck extension.</li><li>Distribution head glass leaks; replace.</li></ul>
	Addition amount of the sodium hydroxide too little; no ammonia development.	<ul style="list-style-type: none"><li>Check the constant flow rate of the NaOH pump (see Technical Data).</li></ul>
	Too low boric acid amount in the receiver; escaping ammonia is not completely bonded.	<ul style="list-style-type: none"><li>Increase of the boric acid amount.</li></ul>
	Tube not completely immersed in the acid receiver.	<ul style="list-style-type: none"><li>Increase of the acid amount.</li></ul>
	Formation of stable ammonia compounds which are not destroyed with sodium hydroxide.	<ul style="list-style-type: none"><li>This problem only occurs with catalysts containing mercury. Sodium sulphate solution destroys these compounds.</li></ul>

## การดูแลบำรุงรักษาเชิงป้องกัน

### Preventive Maintenance



บริษัท ดีเคเอสเอช เทคโนโลยี จำกัด

ฝ่ายบริการหลังการขาย

โทร 0 2 639 7000 E-mail: [service.tec.th@dksh.com](mailto:service.tec.th@dksh.com)

ฝ่ายขายและการตลาด

โทร 0 2 639 7000 E-Mail : [marketing.tec.th@dksh.com](mailto:marketing.tec.th@dksh.com)

Website : [www.dksh.co.th/technology/scientific-thailand](http://www.dksh.co.th/technology/scientific-thailand)

#### เงื่อนไขการให้บริการ Preventive Maintenance

บริษัทฯ จะส่งวิศวกรผู้ชำนาญ เพื่อให้บริการตามขอบข่ายของการบริการ เฉพาะ ในวันและเวลา ราชการ หากมีความประสงค์ที่จะรับบริการนอกเหนือจากวัน เวลา ราชการ (วันหยุดเสาร์ – อาทิตย์ หรือวันหยุด นักชดถุญ) บริษัทฯ จะคิดค่าบริการเพิ่มเติมตามอัตราที่กฎหมายแรงงานกำหนดไว้

#### ขอบข่ายการบริการ

- ตรวจสอบสภาพการทำงานต่าง ๆ ของเครื่องมือ
- ทดสอบประสิทธิภาพการทำงานของเครื่องมือ
- รายการผลการตรวจสอบเครื่องมือ

#### หมายเหตุ

- ราคานี้ไม่รวมถึงค่าบริการซ่อม หรือ เปลี่ยนอะไหล่ที่ชำรุดเสียหาย หรือหมดสภาพการใช้งาน
- ในกรณีที่ผู้รับบริการอยู่นอกเขตพื้นที่ให้บริการ บริษัทฯ จำเป็นต้องคิดค่าใช้จ่ายเพิ่มเติม ได้แก่ ค่าเดินทาง เป็นต้น
- บริษัท ฯ ขอสงวนสิทธิ์ในการเปลี่ยนแปลงราคา โดยไม่แจ้งให้ทราบล่วงหน้า

## ช่องทางการติดต่อ



**DKSH Technology Limited** (บริษัท ดีเคเอสเอช เทคโนโลยี จำกัด)  
เลขที่ 2533 ถนนสุขุมวิท แขวงบางจาก เขตพระโขนง กรุงเทพฯ 10260  
เลขประจำตัวผู้เสียภาษี 010-555-001-4547 (สำนักงานใหญ่)



LINE: @dkshscientific



Call center 0 2 639 7000



DKSH Scientific



[www.dksh.com/scientific-thailand](http://www.dksh.com/scientific-thailand)



[marketing.tec.th@dksh.com](mailto:marketing.tec.th@dksh.com)



@dkshscientific

## Preventive Maintenance Contract

จำนวนในการทำสัญญาบริการ ...1...ครั้งต่อปี

ครั้งที่ ...1... วันที่ 14/05/2025.....

### รายละเอียดผู้รับบริการ

หน่วยงาน	บริษัท ซี.อี.เอ็ม เทคโนโลยี (ไทยแลนด์) จำกัด		
ที่อยู่	219/43 หมู่ 12 ถนนเพชรเกษม ตำบลอ้อมน้อย อำเภอกะทู้มูบแบน จังหวัดสมุทรสาคร 74130		
โทรศัพท์	0869054664	แฟกซ์	-

### ผู้ติดต่อ

ชื่อ - นามสกุล	คุณศิริภาพร พิมพ์				
ตำแหน่ง	เจ้าหน้าที่ห้องปฏิบัติการ				
โทรศัพท์	0869054664	เบอร์ต่อ	-	แฟกซ์	-
E-mail	lab.cemtech1@gmail.com				

### รายละเอียดผู้ให้บริการ

บริษัท ดีเคเอสเอช เทคโนโลยี จำกัด (ฝ่ายบริการหลังการขาย) (สำนักงานใหญ่)

เลขที่ 2533 ถนนสุขุมวิท แขวงบางจาก เขตพระโขนง กรุงเทพฯ 10260

โทรศัพท์ 0 2 693 7000 Email: [jirayut.js@dksh.com](mailto:jirayut.js@dksh.com)

เจ้าหน้าที่ประสานงาน : คุณจิรายุณ สลอาด


เจ้าหน้าที่ผู้ให้บริการ	นายจิรายุณ สลอาด		
ตำแหน่ง	Specialist, Technical Service.		
โทรศัพท์	0938138736	แฟกซ์	-
E-mail	<a href="mailto:jirayut.js@dksh.com">Jirayut.js@dksh.com</a>		

ลงนามผู้รับบริการ		ลงนามผู้ให้บริการ	<i>Jirayut Saly-Ard</i>
ตัวบรรจง	(.....)	ตัวบรรจง	(นาย จิรายุณ สลอาด)
ตำแหน่ง		ตำแหน่ง	Specialist, Technical Service.
วันที่ / ประทับตราบริษัท		วันที่ / ประทับตราบริษัท	14/05/2025

JOB No: WQ-00070598.....MODEL: KT.20s..... S/N: GER5720180118

Part 3: ตรวจเช็คสภาพเครื่อง

Front and rear view of KT-L version

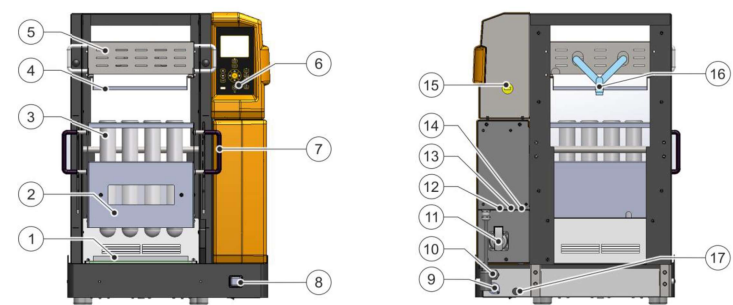

No.		PASS	Fail	N/A	Remark
1	KJELDATHERM digestion block	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	เสื่อมสภาพ
2	Insert rack	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	
3	Digestion tube	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	
4	Stainless steel drip tray	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	
5	Exhaust manifold	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	
6	Controls module, removable	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	
7	Handle for insert rack	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	
8	Mains switch with overcurrent protection function	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	
9	Connection for lift unit	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	
10	Mains cable with plug	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	
11	Power supply for TURBOSOG	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	
12	Connects controller module to block	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	
13	Connection for fan for cooling samples (optional)	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	
14	Connection for external cooling water valve (optional)	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	
15	Connects controller module to block	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	
16	Connection for Iso-Versinic hose (extraction)	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	
17	Excess temperature fuse	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	
18	Lift	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	

Part 4: ละเอียดและรายงานผลการให้บริการ Preventive Maintenance

4.1 ตรวจเช็คระบบไฟฟ้า


	Pass	Fai	N/A	Remark
ใช้ไฟ 220 V/50 Hz	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	.....
กระแสไฟฟ้าตามพิกัดเครื่อง	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	.....

4.2 ตรวจสอบสภาพอุปกรณ์ภายนอก

	Pass	Fail	N/A	Remark
สายไฟของเครื่อง	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	.....
ท่อแก๊วรวมไอกรด	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	.....
สายยางต่อกับท่อแก๊วรวมไอกรด	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	.....
สภาพของ Aluminum block	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	เสื่อมสภาพ
การขึ้นลงของ Lift	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	.....
Light	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	.....
Current Switch	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	.....
Thermostat	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	.....




4.3 ตรวจสอบระบบการทำงาน

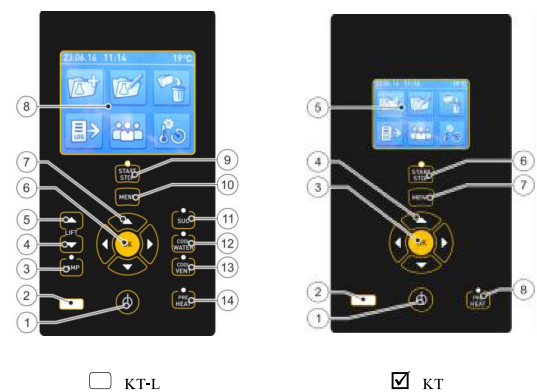

	Pass	Fail	N/A	Remark
Switch controller on or off.	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	.....
USB port	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	.....
LAMP button	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	.....
LIFT down button	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	.....
LIFT up button	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	.....
OK button	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	.....
Navigation buttons	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	.....
Display	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	.....
START/STOP button	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	.....
MENU button	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	.....
SUC button	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	.....
COOLWATER button (optional)	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	.....
COOL VENT button (optional)	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	.....
PRE HEAT button	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	.....
การขึ้นของอุณหภูมิมากกว่า10องศาต่อหน้าที่ที่250องศา	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	.....
การทำงานของตัวป้องกันอุณหภูมิสูงเกิน	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	.....
การทำงานของระบบควบคุมอุณหภูมิ	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	.....

การบำรุงรักษาทั่วไป (Basic maintenance)

- การย่อยตัวอย่างเกิดการเดือดที่รุนแรงอันเนื่องมาตัวอย่างนั้นสามารถป้องกันได้โดยแนะนำให้ย่อยด้วยการตั้งการเพิ่มอุณหภูมิเป็นระดับเช่น ย่อยที่ระดับอุณหภูมิ 250 C ระยะเวลา 15 นาทีจึงเปลี่ยนเป็นอุณหภูมิ 380 C เพื่อป้องกันการล้นออกมา
- เมื่อใช้เสร็จไม่ควรปล่อยให้ Tube เย็นกับตัวเครื่อง
- ต้องนำเอาคลองไอกรดใส่ทุกครั้งหลังจากใช้งานเสร็จ เพื่อป้องกันการหยดของไอกรดที่จะหยดลงมาที่ตัวเครื่อง
- ทำความสะอาดตัวหลุมย่อยด้วยน้ำหรือผ้าชุบน้ำในกรณีที่มีคราบกรดหยดลงมาติดอยู่ในหลุม เพื่อป้องกันไม่ให้คราบดังกล่าวไปกั้นการแผ่อุณหภูมิ



## Certificate of Calibration

Certificate No.: C31250348

Page: 2 of 3

**Equipment:** Cooled Incubator  
**Model:** KB 240  
**Serial No.(or ID):** 20180000012164 ( WW-16-001 )  
**Manufacturer:** Binder  
**Condition:** In Condition  
**Shelves(pc.):** 3

**Certificate No.:** C31250348  
**Issued Date:** 10 February 2025  
**Job No.:** WO-00060640  
**Page:** 1 of 3  
**Ventilation Valve:** Closed

**Customer:** C.E.M Technology (Thailand) Co., Ltd.  
 219/43 Moo 12 Petchkasem Road,  
 Omnoi Krathum Baen, Samut Sakhon 74130 Thailand

**Environment Condition:** Temperature: 22 °C ± 1.8 °C  
 Humidity: 61 %RH ± 5.3 %RH  
 Voltage: 230 VAC ± 1.5 VAC


**Calibration Place:** C.E.M Technology (Thailand) Co., Ltd. ( Laboratory Room )  
 219/43 Moo 12 Petchkasem Road,  
 Omnoi Krathum Baen, Samut Sakhon 74130 Thailand

**Calibration By:** Mr. Tweewong Thaitiang


**Calibration Date:** 10 February 2025

**The Method used:** In house method, CAL-WI-16, base on TLAS-G20

**Traceability:** This certificate is traceable to the SI Units maintained by National Institute of Metrology (NIMT), Thailand through DKSH Technology Limited.  
 Certificate No. C10240018

  
 (Mr. Tweewong Thaitiang)

Person in charge

  
 (Mr. Udon Srichana)  
 Authorized signatory


This certificate is issued the units of measurement according to the International System of Units (SI). It provides traceability of measurement to international or national standard or other recognized national standard laboratories.  
 The measurement uncertainty stated is the expanded uncertainty which is obtained from the standard uncertainty multiplied by the coverage factor (k=2) to provide a level of confidence of approximately 95%. It is determined in accordance with the Guide to Expression of Uncertainty in Measurement (GUM).

These results may be affected by deviations from specified conditions. The results relate only to the items tested, calibrated or sampled. The report shall not be reproduced except in full without approval of DKSH Technology Limited.

บริษัท ดีเคเอส เทคโนโลยี จำกัด  
 DKSH Technology Limited  
 2533 สุขุมวิท 10260 ถนนสุขุมวิท แขวงคลองเตย เขตคลองเตย กรุงเทพมหานคร 10260  
 Phone: +66 2639 7000 Email: info.calibration@dksh.com Website: www.dksh.com/scientific-thailand

Delivering Growth – in Asia and Beyond.

CAL-FM-C31-10: 12 Sep 2022

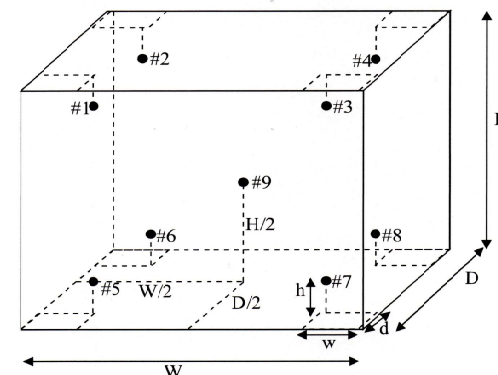

### Standard Installation Locations

Volume (Calibration Zone)= 122 (Liters)

Inside chamber: W = 65 (cm) D = 50 (cm) H = 76 (cm)  
 Standard Locations (#1, #2, #3, #4): w = 7 (cm) d = 5 (cm) h = 8 (cm)  
 Standard Locations (#5, #6, #7, #8): w = 7 (cm) d = 5 (cm) h = 8 (cm)  
 #9: Geometric center of the chamber

Position of Std	#1	#2	#3	#4	#5	#6	#7	#8	#9
Channel of Logger	201	202	203	204	205	206	207	208	209

### Definitions

**Indicating Temperature:** The average reading of indicating device which forms the integral part of the enclosure.

**Measured Temperature:** The average reading of standards at any positions or location.

**Measured Uniformity:** The maximum difference of measured temperatures between of any probes and the measured temperature at the reference location which are observed at same time or at close observation time as possible to determine the temperature pattern or homogeneity with the chamber at steady-state. The reference probe is preferably located in the geometric center of the chamber.

**Measured Stability:** The one-half of greatest maximum difference of measured temperatures at any one probe.

**Overall Variation:** The difference of maximum and minimum measured temperatures throughout observation time.

บริษัท ดีเคเอส เทคโนโลยี จำกัด  
 DKSH Technology Limited  
 2533 สุขุมวิท 10260 ถนนสุขุมวิท แขวงคลองเตย เขตคลองเตย กรุงเทพมหานคร 10260  
 Phone: +66 2639 7000 Email: info.calibration@dksh.com Website: www.dksh.com/scientific-thailand

Delivering Growth – in Asia and Beyond.

CAL-FM-C31-10: 12 Sep 2022



Refer to Certificate No.: C31250348 Page: 1 of 1

### Statements of conformity:

This conformity certificate documents the validity of the following statements of conformity based on the measurement results of corresponding calibration certificate

The correction of indication determined during calibration are under given measurement and environmental conditions and considering the expanded measurement uncertainty (coverage probability 95%) within the specification. The given measurement uncertainty already includes other all effects by according to the standard method, TLAS-G20. Therefore, those parameters have not been assessed separately.

#### Tolerance and Decision rules:

Assessment of the conformity of the measurement device are done based on direct comparison of the relevant measurement results with the tolerances and decision rule are prescribed by the customer.

- Decision rule:**
- ☐ Choice A Binary Statement for Simple Acceptance Rule ( $w = 0$ ), Specific Risk < 50% PFA.
  - ☒ Choice B Non-binary statement with guard band ( $w = 1$  U), Pass or Fail Specific Risk < 2.5% PFA and Condition Pass or Condition Fail Specific Risk < 50% PFA.
  - ☐ Choice C Customer defined, Customers may define arbitrary multiple of  $r$  to have applied as guard band ( $w = r$  U).
- : PFA – Probability of False Accept

(Mr. Udon Srichana)  
Authorized signatory

#### Without adjustment

Desired Temperature : 20.0 °C Tolerances : 1.0 °C

Measurement Temperature at Spread Locations, Indicating of Unit Under Calibration: 20.0 °C

Locations	Measured (°C)	Correction* (°C)	Guard band (W) (± °C)	Tolerance (± °C)	Conformity
#1	20.14	0.14	0.33	1.0	Pass
#2	20.14	0.14	0.34	1.0	Pass
#3	19.96	-0.04	0.38	1.0	Pass
#4	20.14	0.14	0.35	1.0	Pass
#5	20.11	0.11	0.33	1.0	Pass
#6	20.17	0.17	0.34	1.0	Pass
#7	20.00	0.00	0.37	1.0	Pass
#8	20.06	0.06	0.35	1.0	Pass
#9	20.38	0.38	0.33	1.0	Pass

Correction\* = Measured Temperature - Desired Temperature



The validity of the statements of conformity cannot be guaranteed for different places of use, environmental conditions or improper use.

#### The End of Statements of Conformity

บริษัท ดีเคเอสเอช เทคโนโลยี จำกัด  
DKSH Technology Limited  
2533 ถนนสุขุมวิท แขวงคลองเตย เขตคลองเตย กรุงเทพมหานคร 10260  
2533 Sukhumvit Road, Bangkok, Phrakhanong, Bangkok 10260  
Phone: +66 2639 7000 E-mail: info.calibration@dksh.com Website: www.dksh.com/scientific-thailand

Delivering Growth - in Asia and Beyond.

CAL-FM-C31-10: 12 Sep 2022

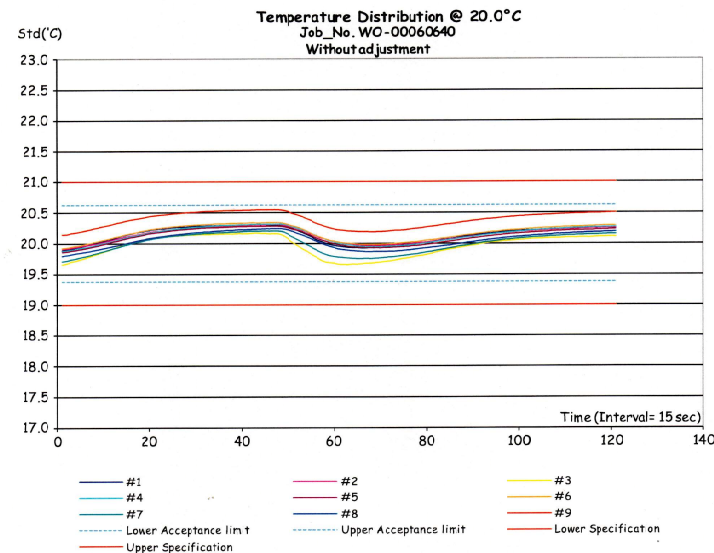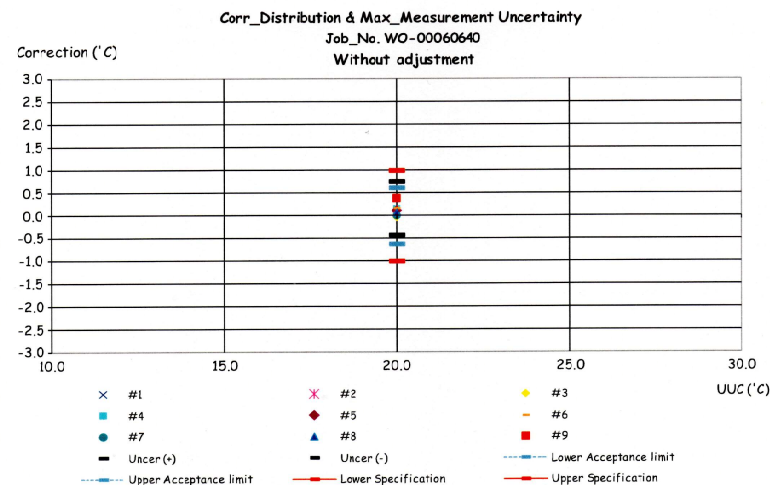

## ใบตรวจสอบสภาพเครื่องควบคุมอุณหภูมิ

เลขที่ใบงาน: WO-00060640

ชนิดเครื่องมือ: Coded Incubator รุ่น: KB 240

หมายเลขเครื่อง: 20180000012164 (WW-16-001)

ตรวจสอบ (รับ)		รายการตรวจเช็ค	ตรวจสอบ (ส่ง)		หมายเหตุ
10 Feb 2025			10 Feb 2025		
ปกติ	ไม่ปกติ		ปกติ	ไม่ปกติ	
		General			
<input checked="" type="checkbox"/>	<input type="checkbox"/>	1. สายไฟ	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	2. การทำงาน Main Switch	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	3. การทำงาน Selector Key	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	4. การแสดงผล Display	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	5. การทำงาน พัดลม	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input type="checkbox"/>	<input type="checkbox"/>	6. สภาพ Lever of Ventilation valve	<input type="checkbox"/>	<input type="checkbox"/>	ไม่มี
<input checked="" type="checkbox"/>	<input type="checkbox"/>	7. สภาพ Lever door open / close	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	8. สภาพ Door seal	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	9. การทำงานของระบบ Safety	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	10. การทำงานของระบบทำความเย็น	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input type="checkbox"/>	<input type="checkbox"/>	11. การทำงานของระบบทำความร้อน	<input type="checkbox"/>	<input type="checkbox"/>	ไม่มี
<input checked="" type="checkbox"/>	<input type="checkbox"/>	12. สภาพตัวเครื่อง	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	13. สภาพแวดล้อม ณ สถานที่ตั้งเครื่อง	<input checked="" type="checkbox"/>	<input type="checkbox"/>	

ข้อแนะนำ:

Mr. Tweewong Thaihiang  
Service Engineer

Certificate No.: C31250348

Page: 3 of 3

### Calibration Results:

Without adjustment

Measurement Temperature at Spread Locations, Indicating of Unit Under Calibration: 20.0 °C

Locations	Measured Temperature (°C)	Correction of UUC. (°C)	Uncertainty (± °C)
#1	20.14	0.14	0.33
#2	20.14	0.14	0.34
#3	19.96	-0.04	0.38
#4	20.14	0.14	0.35
#5	20.11	0.11	0.33
#6	20.17	0.17	0.34
#7	20.00	0.00	0.37
#8	20.06	0.06	0.35
#9	20.38	0.38	0.33

### Temperature Distribution

Desired (°C)	Setting (°C)	Indicating (°C)	Measured Temperature at Spread Locations (°C)									Uncertainty (± °C)*
			#1	#2	#3	#4	#5	#6	#7	#8	#9	
20.0	20.0	20.0	20.14	20.14	19.96	20.14	20.11	20.17	20.00	20.06	20.38	0.38

### Chamber Characterization

Indicating (°C)	Measured Uniformity (°C)	Measured Stability (± °C)	Overall Variation (°C)
20.0	0.57	0.26	0.89

Ncte: \* Maximum uncertainty of the each position

The End of Certificate





## Certificate of Calibration



**Equipment:** Hot Air Oven  
**Model:** UF 55  
**Serial No.(or ID):** B219.0142 ( WW-05-002 )  
**Manufacturer:** Memmert  
**Condition:** In Condition  
**Shelves(pc.):** 2

**Certificate No.:** C31250347  
**Issued Date:** 10 February 2025  
**Job No.:** WO-00060640  
**Page:** 1 of 4  
**Ventilation Valve:** Closed

**Customer:** C.E.M Technology (Thailand) Co., Ltd.  
219/43 Moo 12 Petchkasem Road,  
Omnoi Krathum Baen, Samut Sakhon 74130 Thailand

**Environment Condition:** Temperature: 28 °C ± 1.0 °C  
Humidity: 61 %RH ± 5.3 %RH  
Voltage: 230 VAC ± 1.5 VAC

**Calibration Place:** C.E.M Technology (Thailand) Co., Ltd. ( Laboratory Room )  
219/43 Moo 12 Petchkasem Road,  
Omnoi Krathum Baen, Samut Sakhon 74130 Thailand

**Calibration By:** Mr. Tweewong Thaihang

**Calibration Date:** 10 February 2025

**The Method used:** In house method, CAL-WI-16, base on TLAS-G20

**Traceability:** This certificate is traceable to the SI Units maintained by National Institute of Metrology (NIMT), Thailand through DKSH Technology Limited.  
Certificate No. C10240018

(Mr. Tweewong Thaihang)

Person in charge

(Mr. Udon Srichana)  
Authorized signatory

This certificate is issued the units of measurement according to the International System of Units (SI). It provides traceability of measurement to international or national standard or other recognized national standard laboratories.  
The measurement uncertainty stated is the expanded uncertainty which is obtained from the standard uncertainty multiplied by the coverage factor ( $k=2$ ) to provide a level of confidence of approximately 95%. It is determined in accordance with the Guide to Expression of Uncertainty in Measurement (GUM).  
These results may be affected by deviations from specified conditions. The results relate only to the items tested, calibrated or sampled. The report shall not be reproduced except in full without approval of DKSH Technology Limited.

บริษัท ดีเคเอส อีเซีย จำกัด  
DKSH Technology Limited  
2533 สุขุมวิท 102/2 ถนนสุขุมวิท แขวงคลองเตย เขตคลองเตย กรุงเทพมหานคร 10250  
2533 Sukhumvit Road, Bangkok 10250  
Phone: +66 2639 7000 Email: info.calibration@dksh.com Website: www.dksh.com/scientific-thailand


Delivering Growth - in Asia and Beyond.

CAL-FM-C31-10: 12 Sep 2022



Certificate No.: C31250347

Page: 2 of 4

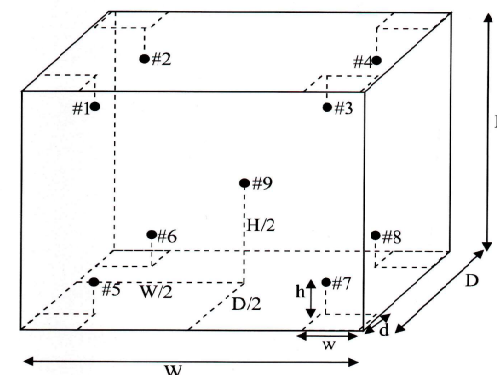

### Standard Installation Locations

Volume (Calibration Zone)= 21 (Liters)

Inside chamber: W = 40 (cm) D = 33 (cm) H = 40 (cm)

Standard Locations (#1, #2, #3, #4): w = 5 (cm) d = 5 (cm) h = 5 (cm)

Standard Locations (#5, #6, #7, #8): w = 5 (cm) d = 5 (cm) h = 5 (cm)

#9: Geometric center of the chamber

Position of Std	#1	#2	#3	#4	#5	#6	#7	#8	#9
Channel of Logger	101	102	103	104	105	106	107	108	109

### Definitions

**Indicating Temperature:** The average reading of indicating device which forms the integral part of the enclosure.

**Measured Temperature:** The average reading of standards at any positions or location.

**Measured Uniformity:** The maximum difference of measured temperatures between of any probes and the measured temperature at the reference location which are observed at same time or at close observation time as possible to determine the temperature pattern or homogeneity with the chamber at steady-state. The reference probe is preferably located in the geometric center of the chamber.

**Measured Stability:** The one-half of greatest maximum difference of measured temperatures at any one probe.

**Overall Variation:** The difference of maximum and minimum measured temperatures throughout observation time.

บริษัท ดีเคเอส อีเซีย จำกัด  
DKSH Technology Limited  
2533 สุขุมวิท 102/2 ถนนสุขุมวิท แขวงคลองเตย เขตคลองเตย กรุงเทพมหานคร 10250  
2533 Sukhumvit Road, Bangkok 10250  
Phone: +66 2639 7000 Email: info.calibration@dksh.com Website: www.dksh.com/scientific-thailand

Delivering Growth - in Asia and Beyond.

CAL-FM-C31-10: 12 Sep 2022





Certificate No.: C31250347

Page: 3 of 4

**Calibration Results:****Without adjustment**

Measurement Temperature at Spread Locations, Indicating of Unit Under Calibration: 104.0 °C

Locations	Measured Temperature (°C)	Correction of UUC. (°C)	Uncertainty (± °C)
#1	104.29	0.29	0.40
#2	104.01	0.01	0.40
#3	104.34	0.34	0.40
#4	104.23	0.23	0.39
#5	104.43	0.43	0.40
#6	104.19	0.19	0.40
#7	103.78	-0.22	0.40
#8	104.21	0.21	0.40
#9	104.47	0.47	0.41

**Temperature Distribution**

Desired (°C)	Setting (°C)	Indicating (°C)	Measured Temperature at Spread Locations (°C)									Uncertainty (± °C)*
			#1	#2	#3	#4	#5	#6	#7	#8	#9	
104.0	104.0	104.0	104.29	104.01	104.34	104.23	104.43	104.19	103.78	104.21	104.47	0.41

**Chamber Characterization**

Indicating (°C)	Measured Uniformity (°C)	Measured Stability (± °C)	Overall Variation (°C)
104.0	0.76	0.18	1.04

Note: \* Maximum uncertainty of the each position



Certificate No.: C31250347

Page: 4 of 4

**Without adjustment (Cont.)**

Measurement Temperature at Spread Locations, Indicating of Unit Under Calibration: 180.0 °C

Locations	Measured Temperature (°C)	Correction of UUC. (°C)	Uncertainty (± °C)
#1	180.20	0.20	0.43
#2	179.54	-0.46	0.43
#3	180.39	0.39	0.43
#4	180.09	0.09	0.43
#5	180.62	0.62	0.43
#6	179.97	-0.03	0.43
#7	179.53	-0.47	0.48
#8	180.27	0.27	0.43
#9	180.57	0.57	0.43

**Temperature Distribution**

Desired (°C)	Setting (°C)	Indicating (°C)	Measured Temperature at Spread Locations (°C)									Uncertainty (± °C)*
			#1	#2	#3	#4	#5	#6	#7	#8	#9	
180.0	xxx	180.0	180.20	179.54	180.39	180.09	180.62	179.97	179.53	180.27	180.57	0.48

**Chamber Characterization**

Indicating (°C)	Measured Uniformity (°C)	Measured Stability (± °C)	Overall Variation (°C)
180.0	1.26	0.19	1.39

Note: \* Maximum uncertainty of the each position

**The End of Certificate**



Refer to Certificate No.: C31250347 Page: 1 of 2

### Statements of conformity:

This conformity certificate documents the validity of the following statements of conformity based on the measurement results of corresponding calibration certificate.

The correction of indication determined during calibration are under given measurement and environmental conditions and considering the expanded measurement uncertainty (coverage probability 95%) within the specification. The given measurement uncertainty already includes other all effects by according to the standard method, TLAS-G20. Therefore, those parameters have not been assessed separately.

#### Tolerance and Decision rules:

Assessment of the conformity of the measurement device are done based on direct comparison of the relevant measurement results with the tolerances and decision rule are prescribed by the customer.

- Decision rule:**
- ☐ Choice A Binary Statement for Simple Acceptance Rule ( $w = 0$ ), Specific Risk < 50% PFA.
  - ☒ Choice B Non-binary statement with guard band ( $w = 1$  U), Pass or Fail Specific Risk < 2.5% PFA and Condition Pass or Condition Fail Specific Risk < 50% PFA.
  - ☐ Choice C Customer defined, Customers may define arbitrary multiple of  $r$  to have applied as guard band ( $w = r$  U).  
; PFA – Probability of False Accept

(Mr. Udon Srichana)  
Authorized signatory

### Without adjustment

Desired Temperature : 104.0 °C Tolerances : 1.0 °C

Measurement Temperature at Spread Locations, Indicating of Unit Under Calibration: 104.0 °C

Locations	Measured (°C)	Correction* (°C)	Guard band (W) (± °C)	Tolerance (± °C)	Conformity
#1	104.29	0.29	0.40	1.0	Pass
#2	104.01	0.01	0.40	1.0	Pass
#3	104.34	0.34	0.40	1.0	Pass
#4	104.23	0.23	0.39	1.0	Pass
#5	104.43	0.43	0.40	1.0	Pass
#6	104.19	0.19	0.40	1.0	Pass
#7	103.78	-0.22	0.40	1.0	Pass
#8	104.21	0.21	0.40	1.0	Pass
#9	104.47	0.47	0.41	1.0	Pass

Correction\* = Measured Temperature - Desired Temperature

The validity of the statements of conformity cannot be guaranteed for different places of use, environmental conditions or improper use.

บริษัท ดีเคเอสเอช เทคโนโลยี จำกัด  
DKSH Technology Limited  
2533 สุขุมวิท Road, Bangkok, Phrakhanong, Bangkok 10260  
Phone: +66 2639 7000 Email: info.calibration@dksh.com Website: www.dksh.com/scientific-thailand

Delivering Growth - in Asia and Beyond.

CAL-FM-C31-10: 12 Sep 2022



Refer to Certificate No.: C31250347 Page: 2 of 2

### Statements of conformity:(Cont.)

#### Without adjustment (Cont.)

Desired Temperature : 180.0 °C Tolerances : 2.0 °C

Measurement Temperature at Spread Locations, Indicating of Unit Under Calibration: 180.0 °C

Locations	Measured (°C)	Correction* (°C)	Guard band (W) (± °C)	Tolerance (± °C)	Conformity
#1	180.20	0.20	0.43	2.0	Pass
#2	179.54	-0.46	0.43	2.0	Pass
#3	180.39	0.39	0.43	2.0	Pass
#4	180.09	0.09	0.43	2.0	Pass
#5	180.62	0.62	0.43	2.0	Pass
#6	179.97	-0.03	0.43	2.0	Pass
#7	179.53	-0.47	0.48	2.0	Pass
#8	180.27	0.27	0.43	2.0	Pass
#9	180.57	0.57	0.43	2.0	Pass

Correction\* = Measured Temperature - Desired Temperature




The validity of the statements of conformity cannot be guaranteed for different places of use, environmental conditions or improper use.

The End of Statements of Conformity

บริษัท ดีเคเอสเอช เทคโนโลยี จำกัด  
DKSH Technology Limited  
2533 สุขุมวิท Road, Bangkok, Phrakhanong, Bangkok 10260  
Phone: +66 2639 7300 Email: info.calibration@dksh.com Website: www.dksh.com/scientific-thailand

Delivering Growth - in Asia and Beyond.

CAL-FM-C31-10: 12 Sep 2022

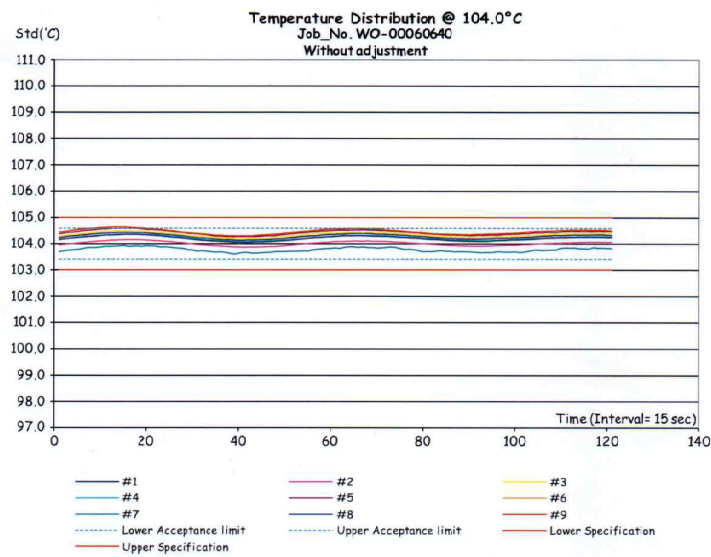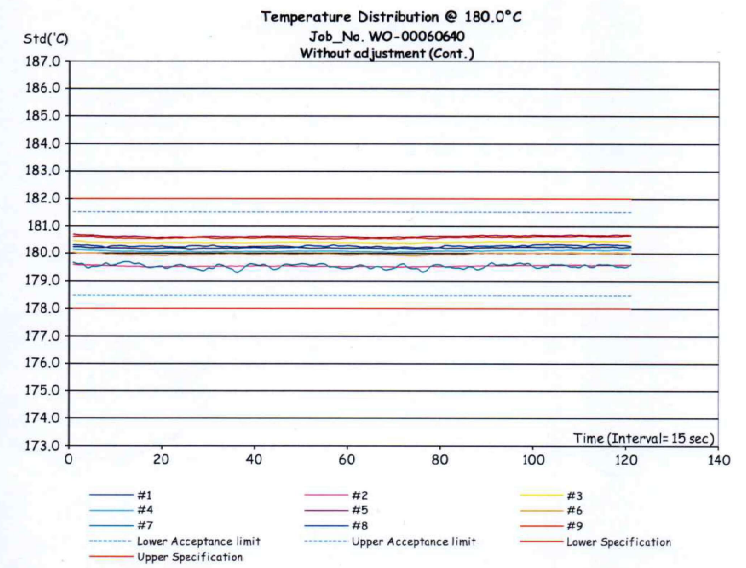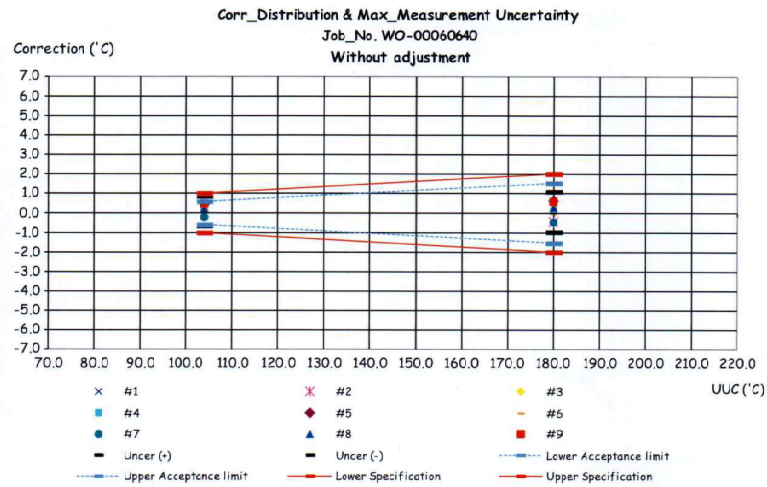





## ใบตรวจสอบสภาพเครื่องควบคุมอุณหภูมิ

เลขที่ใบงาน: WO-00060640

ชนิดเครื่องมือ: Hot Air Oven

รุ่น: UF 55

หมายเลขเครื่อง: B219.0142 ( WW-05-002 )

ตรวจสอบ (รับ)		รายการตรวจเช็ค	ตรวจสอบ (ส่ง)		หมายเหตุ
10 Feb 2025			10 Feb 2025		
ปกติ	ไม่ปกติ		ปกติ	ไม่ปกติ	
		General			
<input checked="" type="checkbox"/>	<input type="checkbox"/>	1. สายไฟ	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	2. การทำงาน Main Switch	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	3. การทำงาน Selector Key	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	4. การแสดงผล Display	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	5. การทำงาน ฟัดลม	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	6. สภาพ Lever of Ventilation valve	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	7. สภาพ Lever door open / close	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	8. สภาพ Door seal	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	9. การทำงานของระบบ Safety	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input type="checkbox"/>	<input type="checkbox"/>	10. การทำงานของระบบทำความเย็น	<input type="checkbox"/>	<input type="checkbox"/>	ไม่มี
<input type="checkbox"/>	<input type="checkbox"/>	11. การทำงานของระบบทำความร้อน	<input type="checkbox"/>	<input type="checkbox"/>	ไม่มี
<input checked="" type="checkbox"/>	<input type="checkbox"/>	12. สภาพตัวเครื่อง	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	13. สภาพแวดล้อม ณ สถานที่ตั้งเครื่อง	<input checked="" type="checkbox"/>	<input type="checkbox"/>	

ข้อแนะนำ :

Mr. Tweewong Thaihiang  
Service Engineer

บริษัท ดีเคเอสเอช (ประเทศไทย) จำกัด  
DKSH Technology Limited  
2533 ถนนสุขุมวิท แขวงบางจาก เขตพระโขนง กรุงเทพมหานคร 10260  
2533 Sukhumvit Road, Bangchak, Phraekhanong Bangkok 10260  
Phone: +66 2639 7000 Email: info.calibration@dksh.com Website: www.dksh.com/scientific-thailand

Delivering Growth - in Asia and Beyond.

# CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhaprachasan 3 Rd., Bangpoed, Fakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech\_cal@yahoo.com, calibratech\_cal@hotmail.com



NSC-TISI-TIS17225  
CALIBRATION 0030

## Certificate of Calibration

Certificate No. : 68-400089-3

Page : 1 of 2

Submitted by :

C.E.M Technology (Thailand) Co.,Ltd.

219/43 Moo.12 Petchkasem Rd, Omnoi, Krathumban, Samutsakorn 74130 (Head Office)

Equipment :

Temperature Indicator with Thermistor Probe

Temperature Indicator

Manufacturer : Apera

Model : PC 910

Range : N/A °C

Resolution : 0.1 °C

Serial No. : PC910X1220811001

ID No. : WW-03-002

Thermistor probe

Model : N/A

Sheath Material : Stainless

Diameter : 4.8 mm.

Length : 100 mm.

Serial No. : N/A

ID No. : WW-03-002

Environment :

On site calibration was carried out at the Laboratory,

C.E.M Technology (Thailand) Co., Ltd.

Ambient Temperature : (26.0 to 27.0) °C

Relative Humidity : (45 to 50) %

Line Voltage : (224.5 to 226.0) VAC

Date of Received :

11 February 2025

Date of Calibration :

11 February 2025

Date of Issue :

17 February 2025

Calibrated by :

Pernpon Chanpu

Calibration Method :

This instrument was calibrated by In-house method comparison technique CAL-M4003 by compared with PRT in the liquid bath at the constant controlled temperature.

The temperature scale used was based on ITS-90

Reference Standard Instruments :

This certification is traceable to the International System of Units

1. Platinum Resistance Thermometer (PRT)

ID No.

Cert. No.

Due Date

Traceability

400002

TT-0095-24 01 Jul 2026

National Institute of Metrology Thailand (NIMT)

2. Standard Digital Thermometer

ID No.

Cert. No.

Due Date

Traceability

400033

24E633

21 Feb 2026

National Institute of Metrology Thailand (NIMT)

Approved by :

( Pernpon Chanpu )

Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.

CAL-F0031-03



# CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhaphrachasan 3 Rd., Bangpood, Pakkred, Nonhlaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech.cal@yahoo.com, calibratech.cal@hotmail.com

## Certificate of Calibration

Certificate No. : 68-400089-3

Page : 2 of 2

Result of Calibration : Without Adjustment

LUC Condition As-Received : Good

Function : Temperature measurement

Immersion Depth ( mm. )	Standard Reading ( °C )	UUC Reading ( °C )	Correction ( °C )	Uncertainty ( ± °C )
100	25.003	25.2	-0.2	0.19

### Remark

UUC : Unit Under Calibration

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor  $k = 2$ , providing a level of confidence of approximately 95%

- 000 -



CAL-F0031-03

# CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhaphrachasan 3 Rd., Bangpood, Pakkred, Nonhlaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech.cal@yahoo.com, calibratech.cal@hotmail.com



## Certificate of Calibration

Certificate No. : 68-420017-3

Page : 1 of 2

Submitted by : C.E.M Technology (Thailand) Co., Ltd.

219/43 Moo.12 Petchkasem Rd, Omnoi, Krathumban, Samutsakorn 74130 (Heac Office)

Equipment : pH Meter with electrode

pH meter

Manufacturer : Apera

Model : PC 910

Range : N/A

pH

Resolution : 0.01 pH

Serial No. : PC910X1220811001

ID No. : WW-03-002

Electrode

Model : LabSen 211

Serial No. : 2110009/213

ID No. : WW-03-002

Environment : On site calibration was carried out at the Laboratory,

C.E.M Technology (Thailand) Co., Ltd.

Ambient Temperature : (26.0 to 27.0) °C

Relative Humidity : (45 to 50) %

Date of Received : 11 February 2025

Date of Calibration : 11 February 2025

Date of Issue : 17 February 2025

Calibrated by : Permpon Chanpu

Calibration Method : In-house method CAL-M4201 direct measurement by using standard voltage calibrator and using certified reference material (CRM)

Reference Standard Instruments : This certification is traceable to the International System of Units

1. Multiproduct Calibrator

ID No.	Cert. No.	Due Date	Traceability
400005	SG-E-00307/66	23 Aug 2025	National Institute of Metrology Thailand (NIMT)

2. Standard Buffer Solution

pH	Cert. No.	Lot No.	Exp. Date	Traceability
4.008	61293328	1027612	15 Sep 2025	CPA Chem Ltd. Accredited to ISO 17034 and ISO/IEC 17025
6.987	61297593	1027614	15 Sep 2025	CPA Chem Ltd. Accredited to ISO 17034 and ISO/IEC 17025
10.010	61306165	1027613	15 Sep 2025	CPA Chem Ltd. Accredited to ISO 17034 and ISO/IEC 17025

Approved by :

( Permpon Chanpu )

Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



CAL-F0031-03



# CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhprachasan 3 Rd., Bangpoo, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech.cal@yahoo.com, calibratech.cal@hotmail.com

## Certificate of Calibration

Certificate No. : 68-420017-3

Page : 2 of 2

### Result of Calibration :

UUC Condition As-Received : Good

Function : Electrical measurement

pH meter

Performing standard curve by Multiproduct Calibrator at pH (4,7,10)

Adjustment Curve at nominal pH	Applied Voltage ( mV )	Nominal Value ( pH )	UUC Reading		Correction ( mV )	Uncertainty ( ± mV )
			( pH )	( mV )		
4, 7, 10	177.4800	4	4.00	177	0	0.59
	0.0000	7	7.00	0	0	0.58
	-177.4800	10	10.00	-178	1	0.59

Function : pH meter with electrode

Performing a three - buffer standard curve using buffer nominal pH (4,7,10)

Adjustment Curve at nominal pH	Standard Buffer ( pH )	UUC Reading ( pH )	Correction ( pH )	Uncertainty ( ± pH )
4, 7, 10	4.008	4.00	0.01	0.0097
	6.987	7.00	-0.01	0.011
	10.010	10.01	0.00	0.014

### Remark

UUC : Unit Under Calibration

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor  $k = 2$ , providing a level of confidence of approximately 95%

- o O o -



CAL-F0031-03

# CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhprachasan 3 Rd., Bangpoo, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech.cal@yahoo.com, calibratech.cal@hotmail.com

## Certificate of Calibration



NSC-TISI-TIS 17025  
CALIBRATION 0030

Certificate No. : 68-430004-2

Page : 1 of 2

### Submitted by :

C.E.M Technology (Thailand) Co., Ltd.

219/43 Moo 12 Petchkasem Rd, Omnoi, Krathumban, Samutsakorn 74130 (Head Office)

### Equipment :

Digital Conductivity meter with probe

Manufacturer : Apera Model : PC 910

Serial No. : PC910X1220811001 ID No. : WW-03-002

Electrode

Model : N/A Serial No. : N/A

ID No. : WW-03-002

### Environment :

On site calibration was carried out at the Laboratory.

C.E.M Technology (Thailand) Co., Ltd.

Ambient Temperature (26.0 to 27.0) °C

Relative Humidity (45 to 50) %

Date of Received : 11 February 2025

Date of Calibration : 11 February 2025

Date of Issue : 17 February 2025

Calibrated by : Permon Chanpu

Calibration Method : In-house method CAL-M4301 direct measurement by conductivity buffer solution

Reference Standard Instruments : This certification is traceable to the International System of Units

### Standard Buffer Solution

Material	Lot No.	Exp. Date	Traceability
84 µS/cm	0300	01 June 2027	National Institute of Standards and Technology (NIST), U.S.A., S.R.M.
1413 µS/cm	970986	25 April 2025	CPA Chem Ltd. Accredited to ISO 17034 and ISO/IEC 17025
12.88 mS/cm	970987	25 April 2025	CPA Chem Ltd. Accredited to ISO 17034 and ISO/IEC 17025

Approved by :

( Permon Chanpu )

Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



CAL-F0031-03

## Certificate of Calibration

Certificate No. : 68-430004-2

Page : 2 of 2

### Result of Calibration :

UUC Condition As-Received : Good

Function : Conductivity measurement

Before Adjustment

Standard Conductivity Solution	UUC Reading	Correction	Uncertainty ( ± )	Unit
84*	81.9	2.1	1.1	µS/cm
1413	1444	-31	9.0	µS/cm
12.88	12.41	0.47	0.082	mS/cm

After Adjustment : at 25.000, 84, 147, 1413 µS/cm 12.880, 80, 111.80 mS/cm

Standard Conductivity Solution	UUC Reading	Correction	Uncertainty ( ± )	Unit
84*	84.0	0.0	1.1	µS/cm
1413	1413	0	9.0	µS/cm
12.88	12.88	0.00	0.082	mS/cm

### Remark

UUC : Unit Under Calibration

\* This parameter are out of accreditation's scope.

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k = 2,

providing a level of confidence of approximately 95%

- 00 -



## Certificate of Calibration

Certificate No. : 68-400089-1

Page : 1 of 2

### Submitted by :

C.E.M Technology (Thailand) Co.,Ltd.  
219/43 Moo.12 Petchkasem Rd, Omnoi, Krathumban, Samutsakorn 74130 (Head Office)

### Equipment :

Temperature Indicator with Thermistor Probe  
Temperature Indicator  
Manufacturer : Thermo Scientific Model : VERSA STAR PRO  
Range : N/A °C Resolution : 0.1 °C  
Serial No. : 12260 ID No. : WW-03-001  
Thermistor probe  
Model : N/A Sheath Material : Stainless  
Diameter : 6.5 mm. Length : 120 mm.  
Serial No. : PT1-18812 ID No. : WW-03-001

### Environment :

On site calibration was carried out at the Laboratory,  
C.E.M Technology (Thailand) Co., Ltd.  
Ambient Temperature : (26.0 to 27.0) °C  
Relative Humidity : (45 to 50) %  
Line Voltage : (224.5 to 226.0) VAC

Date of Received : 11 February 2025

Date of Calibration : 11 February 2025

Date of Issue : 17 February 2025

Calibrated by : Permpon Chanpu

Calibration Method : This instrument was calibrated by In-house method comparison technique CAL-M4003 by compared with PRT in the dry-well calibrator at the constant controlled temperature.

The temperature scale used was based on ITS-90

Reference Standard Instruments : This certification is traceable to the International System of Units

1. Platinum Resistance Thermometer (PRT)

ID No.	Cert. No.	Due Date	Traceability
400002	TT-0095-24	01 Jul 2026	National Institute of Metrology Thailand (NIMT)

2. Standard Digital Thermometer

ID No.	Cert. No.	Due Date	Traceability
400033	24E633	21 Feb 2026	National Institute of Metrology Thailand (NIMT)

Approved by :   
( Permpon Chanpu )  
Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



# CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhaphrachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech.cal@yahoo.com, calibratech.cal@hotmail.com

## Certificate of Calibration

Certificate No. : 68-400089-1

Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Function : Temperature measurement

Immersion Depth ( mm. )	Standard Reading ( °C )	UUC Reading ( °C )	Correction ( °C )	Uncertainty ( ± °C )
130	25.004	25.1	-0.1	0.19

### Remark

UUC : Unit Under Calibration

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor  $k = 2$ , providing a level of confidence of approximately 95%

- 000 -



CAL-F0031-03

# CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhaphrachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech.cal@yahoo.com, calibratech.cal@hotmail.com



## Certificate of Calibration

Certificate No. : 68-420017-1

Page : 1 of 2

Submitted by : C.E.M Technology (Thailand) Co., Ltd.

219/43 Moo.12 Petchkasem Rd, Omnoi, Krathumbur, Samutsakorn 74130 (Head Office)

Equipment : pH Meter with electrode

pH meter

Manufacturer : Thermo Scientific Model : VERSA STAR PRO

Range : N/A pH Resolution : 0.01 pH

Serial No. : 12260 ID No. : WW-03-001

Electrode

Model : 9156BNWP Serial No. : VV1-15843

ID No. : WW-03-001

Environment : On site calibration was carried out at the Laboratory,

C.E.M Technology (Thailand) Co., Ltd.

Ambient Temperature : (26.0 to 27.0) °C

Relative Humidity : (45 to 50) %

Date of Received : 11 February 2025

Date of Calibration : 11 February 2025

Date of Issue : 17 February 2025

Calibrated by : Permpon Chanpu

Calibration Method : In-house method CAL-M4201 direct measurement by using standard voltage calibrator and using certified reference material (CRM)

Reference Standard Instruments : This certification is traceable to the International System of Units

1. Multiproduct Calibrator

ID No.	Cert. No.	Due Date	Traceability
400005	SG-E-00307/66	23 Aug 2025	National Institute of Metrology Thailand (NIMT)

2. Standard Buffer Solution

pH	Cert. No.	Lot No.	Exp. Date	Traceability
4.008	61293328	1027612	15 Sep 2026	CPA Chem Ltd. Accredited to ISO 17034 and ISO/IEC 17025
6.987	61297593	1027614	15 Sep 2025	CPA Chem Ltd. Accredited to ISO 17034 and ISO/IEC 17025
10.010	61306165	1027613	15 Sep 2025	CPA Chem Ltd. Accredited to ISO 17034 and ISO/IEC 17025

Approved by :

( Permpon Chanpu )

Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



CAL-F0031-03



## Certificate of Calibration

Certificate No. : 68-420017-1

Page : 2 of 2

### Result of Calibration :

UUC Condition As-Received : Good

Function : Electrical measurement

pH meter

Performing standard curve by Multiproduct Calibrator at pH (4,7,10)

Adjustment Curve at nominal pH	Applied Voltage ( mV )	Nominal Value ( pH )	UUC Reading		Correction ( mV )	Uncertainty ( ± mV )
			( pH )	( mV )		
4, 7, 10	177.4800	4	4.00	177.4	0.1	0.12
	0.0000	7	7.00	0.0	0.0	0.086
	-177.4800	10	10.00	-177.4	-0.1	0.12

Function : pH meter with electrode

Performing a three - buffer standard curve using buffer nominal pH (4,7,10)

Adjustment Curve at nominal pH	Standard Buffer ( pH )	UUC Reading ( pH )	Correction ( pH )	Uncertainty ( ± pH )
4, 7, 10	4.008	4.01	0.00	0.0097
	6.987	7.00	-0.01	0.011
	10.010	10.01	0.00	0.014

### Remark

UUC : Unit Under Calibration

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor  $k = 2$ , providing a level of confidence of approximately 95%

- 000 -

+



## Certificate of Calibration

Certificate No. : 68-400089-1

Page : 1 of 2

Submitted by :

C.E.M Technology (Thailand) Co.,Ltd.  
219/43 Moo.12 Petchkasem Rd, Omnoi, Krathumban, Samutsakorn 74130 (Head Office)

Equipment :

Temperature Indicator with Thermistor Probe  
Temperature Indicator  
Manufacturer : Thermo Scientific Model : VERSA STAR PRO  
Range : N/A °C Resolution : 0.1 °C  
Serial No. : 12260 ID No. : WW-03-001  
Thermistor probe  
Model : N/A Sheath Material : Stainless  
Diameter : 6.5 mm. Length : 120 mm.  
Serial No. : PT1-18812 ID No. : WW-03-001

Environment :

On site calibration was carried out at the Laboratory,  
C.E.M Technology (Thailand) Co., Ltd.  
Ambient Temperature : (26.0 to 27.0) °C  
Relative Humidity : (45 to 50) %  
Line Voltage : (224.5 to 226.0) VAC

Date of Received :

11 February 2025

Date of Calibration :

11 February 2025

Date of Issue :

17 February 2025

Calibrated by :

Permpoon Chanpu

Calibration Method : This instrument was calibrated by In-house method comparison technique CAL-M4003 by compared with PRT in the dry-well calibrator at the constant controlled temperature.

The temperature scale used was based on ITS-90

Reference Standard Instruments : This certification is traceable to the International System of Units

1. Platinum Resistance Thermometer (PRT)

ID No.	Cert. No.	Due Date	Traceability
400002	TT-0095-24	01 Jul 2026	National Institute of Metrology Thailand (NIMT)

2. Standard Digital Thermometer

ID No.	Cert. No.	Due Date	Traceability
400033	24E633	21 Feb 2026	National Institute of Metrology Thailand (NIMT)

Approved by :   
( Permpoon Chanpu )  
Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



# CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Suichapachasan 3 Rd., Bangpood, Pakkred, Northaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech.cal@yahoo.com, calibratech.cal@hotmail.com

## Certificate of Calibration

Certificate No. : 68-400089-1

Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Function : Temperature measurement

Immersion Depth ( mm. )	Standard Reading ( °C )	UUC Reading ( °C )	Correction ( °C )	Uncertainty ( ± °C )
130	25.004	25.1	-0.1	0.19

### Remark

UUC : Unit Under Calibration

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor  $k = 2$ , providing a level of confidence of approximately 95%

- 000 -



CAL-F0031-03



THAI CALIBRATION SERVICES CO., LTD.

19/8 Moo 9 Soi Raiking 30 Puttamonthon 5 Rd., Sampran, Nakornpatom 73210

Tel. 0-3439-7682-5 Fax: 0-3439-7687

www.thaical.com E-mail : sale@thaicalibration.com, lab@thaicalibration.com



NSC-TISI-TIS 17025  
CALIBRATION 0189

## CALIBRATION CERTIFICATE

Certificate No.S2503003S

page 1 of 2

**Customer :** C.E.M TECHNOLOGY (THAILAND) CO., LTD.  
219/43 Moo 12 Petchkasem Road, Omnoi,  
Krathumban, Samutsakorn 74130

**Equipment :** Non-automatic weighing instrument (Electronic instrument)  
**Manufacturer :** Sartorius  
**Model :** BSA224S-CW  
**Accuracy class :** -  
**Capacity :** 220 g  
**Resolution :** 0.0001 g  
**Serial No. :** 3139614148  
**ID No. :** CI-01-003  
**Place of calibration :** ห้องเครื่องวัด

**Order No. :** 68S0877-1  
**Ambient temperature :** (20.2 ± 5.0) °C  
**Relative humidity :** (54.5 ± 10.0) %  
**Received date :** 01-Mar-2025  
**Date of calibration :** 01-Mar-2025  
**Date of issue :** 01-Mar-2025  
**Condition of the balance :** Good working conditions

### Calibration method

This instrument was calibrated according to the EURAMET Calibration Guide No. 18.

### Condition of reference standard weight

Instrument	Nominal value	Serial No.	Certificate No.	Due date	Density (kg/m <sup>3</sup> )
1 Standard weight set	1 mg to 2 kg	15885+15849	M24100015	5-Oct-2025	7950

### Traceability of the reference standard weight

This certificate is traceable to SI unit through Mass Calibration Laboratory Thai Calibration Services Co., Ltd., NSC-ONSC accredited no. Calibration 0189.

Calibrated By : Sathaporn Rueangpluppla  
Technician

Approved Signatory :   
Somwang Wongduang

This calibration certificate may not be reproduced other than in full,  
except with the prior written approval of the head of TCS calibration laboratory.

TCS-F-138 Issue 01/Rev.01/12 Jun 2023

NO. 42531





# THAI CALIBRATION SERVICES CO., LTD.

19/8 Moo 9 Soi Raiking 30 Puttamonthon 5 Rd., Sampran, Nakornpatom 73210

Tel. 0-3439-7682-5 Fax: 0-3439-7687

www.thaical.com E-mail : sale@thaicalibration.com, lab@thaicalibration.com



## CALIBRATION CERTIFICATE

Certificate No.S2503003S


page 2 of 2

### The repeatability of indication

Nominal Value (g)	Standard Deviation of reading (g)	Maximum difference between successive reading (g)	n
200	0.0000	0.0000	5

### The effect of eccentric application of a load on the indication (test load : 100 g)

Position	Balance Reading (g)
Point 1	100.0000
Point 2	100.0000
Point 3	99.9999
Point 4	99.9998
Point 5	100.0000
Eccentric Value	0.0002



### The error of indication

Nominal Value (g)	Value of Reference Standard Weight (g)	Balance Reading (g)	Correction (g)	Uncertainty (±) (g)	k
Unload	0.0000	0.0000	0.0000	0.000082	2.00
1	1.0000	1.0000	0.0000	0.000085	2.00
2	2.0000	2.0000	0.0000	0.000087	2.00
5	5.0000	5.0001	-0.0001	0.000090	2.00
10	10.0000	10.0000	0.0000	0.000094	2.00
20	20.0000	20.0000	0.0000	0.00011	2.00
50	50.0000	50.0000	0.0000	0.00013	2.00
100	100.0000	100.0000	0.0000	0.00019	2.00
120	120.0000	120.0001	-0.0001	0.00024	2.00
150	150.0000	150.0000	0.0000	0.00027	2.00
200	200.0002	200.0000	+0.0002	0.00033	2.00

Remark : Adjustment, Internal weight

### Uncertainty of measurement

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor (k), which for a normal distribution corresponds to a coverage probability of approximately 95% (confidence level).

This report will certify of the calibrated equipment only.

--End--



# THAI CALIBRATION SERVICES CO., LTD.

19/8 Moo 9 Soi Raiking 30 Puttamonthon 5 Rd., Sampran, Nakornpatom 73210

Tel. 0-3439-7682-5 Fax: 0-3439-7687

www.thaical.com E-mail : sale@thaicalibration.com, lab@thaicalibration.com



## CALIBRATION CERTIFICATE

Certificate No.S2505043S

page 1 of 2

### Customer :

C.E.M. TECHNOLOGY (THAILAND) CO., LTD.

219/43 Moo 12, Petchkasem Rd., Omnoi,

Krathumban, Samutsakorn 74130

### Equipment :

Non-automatic weighing instrument (Electronic instrument)

### Manufacturer :

Sartorius

### Order No. :

68S1799-1

### Model :

QUINTIX224-1S

### Ambient temperature :

(23.9 ± 1.0) °C

### Accuracy class :

-

### Relative humidity :

(38.9 ± 5.0) %

### Capacity :

220000 mg

### Received date :

30-Apr-2025

### Resolution :

0.1 mg

### Date of calibration :

30-Apr-2025

### Serial No. :

0035009070

### Date of issue :

03-May-2025

### ID No. :

CI-01-002

### Condition of the balance :

Good working conditions

### Place of calibration :

ห้องเครื่องชั่ง

### Calibration method

This instrument was calibrated according to the EURAMET Calibration Guide No. 18.

### Condition of reference standard weight

Instrument	Nominal value	Serial No.	Certificate No.	Due-date	Density (kg/m <sup>3</sup> )
1 Standard weight set	1 mg to 2 kg	15885+15849	M2410001S	5-Oct-2025	7950

### Traceability of the reference standard weight

This certificate is traceable to SI unit through Mass Calibration Laboratory Thai Calibration Services Co., Ltd., NSC-ONSC accredited no. Calibration 0189.

Calibrated By :

Aekhasak Silart

Technician

Approved Signatory :

Somwang Wongduang

This calibration certificate may not be reproduced other than in full,  
except with the prior written approval of the head of TCS calibration laboratory.

**THAI CALIBRATION SERVICES CO., LTD.**

19/8 Moo 9 Soi Raiking 30 Puttamonthon 5 Rd., Sampran, Nakornpatom 73210

Tel. 0-3439-7682-5 Fax: 0-3439-7687

www.thaical.com E-mail : sale@thaicalibration.com, lab@thaicalibration.com

**CALIBRATION CERTIFICATE**

Certificate No.S2505043S


page 2 of 2

**The repeatability of indication**

Nominal Value ( mg )	Standard Deviation of reading ( mg )	Maximum difference between successive reading ( mg )	n
200000	0.04	0.1	5

**The effect of eccentric application of a load on the indication (test load : 100000 mg)**

Position	Balance Reading ( mg )
Point 1	99999.8
Point 2	99999.8
Point 3	99999.8
Point 4	99999.6
Point 5	99999.6
Eccentric Value	0.2

**The error of indication**

Nominal Value ( mg )	Value of Reference Standard Weight ( mg )	Balance Reading ( mg )	Correction ( mg )	Uncertainty (±) ( mg )	k
Unload	0.0	0.0	0.0	0.14	2.21
100	100.0	100.0	0.0	0.14	2.21
200	200.0	200.1	-0.1	0.14	2.21
500	500.0	500.0	0.0	0.14	2.20
1000	1000.0	1000.0	0.0	0.14	2.20
2000	2000.0	2000.0	0.0	0.14	2.20
5000	5000.0	5000.1	-0.1	0.14	2.18
10000	10000.0	10000.0	0.0	0.14	2.16
20000	20000.0	20000.0	0.0	0.15	2.13
50000	50000.0	50000.0	0.0	0.16	2.08
100000	100000.0	99999.8	+0.2	0.21	2.00
200000	200000.2	199999.7	+0.5	0.34	2.00

Remark : Without adjustment

**Uncertainty of measurement**

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor ( $k$ ), which for a normal distribution corresponds to a coverage probability of approximately 95% (confidence level).

**This report will certify of the calibrated equipment only.**

--End--