

TSP HIGH VOLUME AIR SAMPLER CALIBRATION REPORT

Sampler Location				Date	December 9, 2022
Project Site				Start Time	10:30 AM
Sampler Number	TSP No.2	Transfer Standard Type	Orifice	Stop Time	10:45 AM
Motor Serial Number	TSP No.2	Calibrator Model	25A	Person	Mr.Pasagorn Samol
Recorder Serial Number	-	Calibrator Serial Number	307N		


Plate No.	(Delta H)			(A)	(X)	(I)	(Y)	Temperature	Barometric Pressure	Start Meter	Stop Meter
	Positive	Negative	ΔH_{H_2O}	$[\Delta H_{H_2O} (Pa/P_{std}) (T_{std}/T_a)]^{1/2}$	$Q_{std} = (1/m) [(A-b)]$ (m ³ /min)	Sample Flow Rate Indicator (ft ³ /min)	$[C = I [(Pa/P_{std}) (T_{std}/T_a)]^{1/2}]$	(°K = °C+273)	(mmHg)		
5	1.5	1.4	2.9	1.67421	0.82660	36.0	35.70	303.0	760.0		
7	2.0	1.8	3.8	1.94336	0.95703	43.0	42.64	303.0	760.0		
10	3.4	3.3	6.7	2.56124	1.25646	50.0	49.59	303.0	760.0		
13	4.0	3.9	7.9	2.78917	1.36692	55.0	54.54	303.0	760.0		
18	5.5	5.4	10.9	3.26965	1.59976	60.0	59.50	303.0	760.0		

Linear Regression Y ON X : Y= mX + b

1	Slope (m)	2.06353	Linear Equation		Average	303.0	760.0		
2	Intercept (b)	-0.03151	Set Point Flow Rate (X) (m ³ /min)	1.133	r ²	0.999555	Pstd(mmHg)	760.0	
3	Correlation Coefficient (r)	0.99993	Final Set Flow Rate = (I)	0	r	0.9997775	T _{NTP}	298.0	
Result								C=(Pa/Pstd)*(Tstd/Ta)^0.5	0.991714853

COMMENT

Andersen Instruments, Inc.

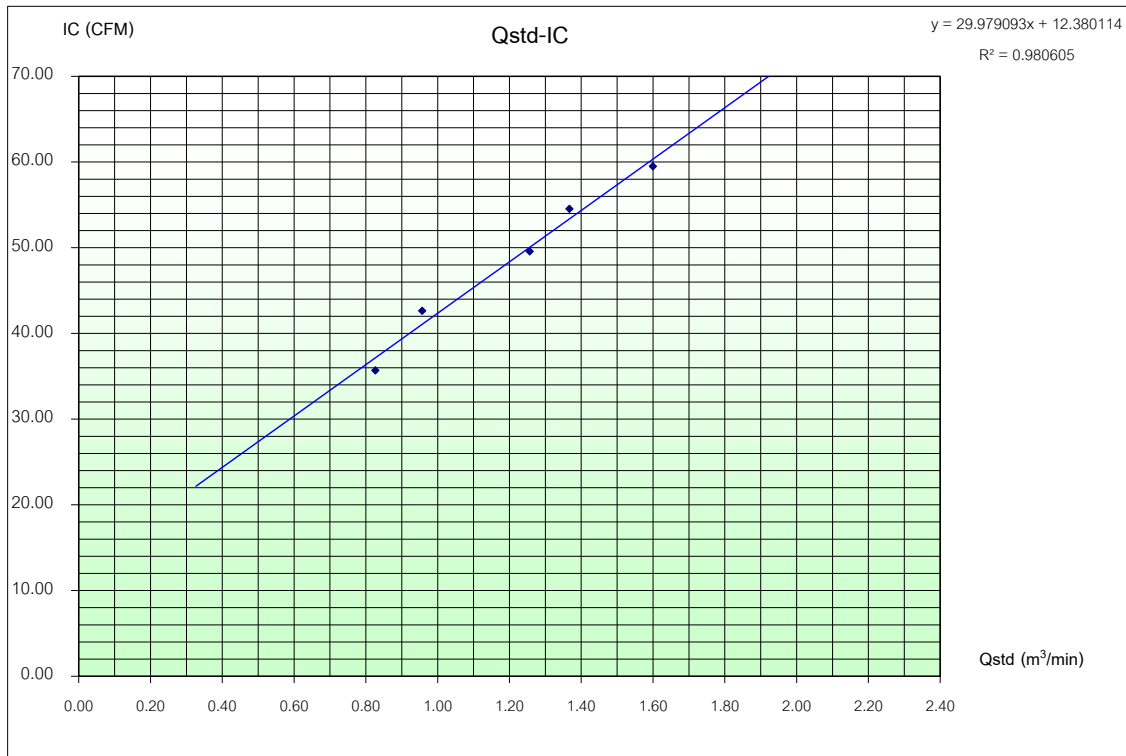

Calibrated By


Mr. Pasagorn Samol

PM10 HIGH VOLUME AIR SAMPLER CALIBRATION REPORT

Sampler Location				Date	December 9, 2022
Project Site				Start Time	10:20 AM
Sampler Number	PM10 No.2	Transfer Standard Type	Orifice	Stop Time	10:35 AM
Motor Serial Number	PM10 No.2	Calibrator Model	25A	Person	Mr.Pasagorn Samol
Recorder Serial Number	-	Calibrator Serial Number	307N		


Plate No.	(Delta H)			(A)	(X)	(I)	(Y)	Temperature	Barometric Pressure	Start Meter	Stop Meter
	Pressure Drop Across Orifice (inH ₂ O)			$[\Delta H_2O(Pa/P_{std})(T_{std}/T_a)]^{1/2}$	$Q_{std} = (1/m)[(A-b)]$	Sample Flow Rate Indication	$IC = I[(Pa/P_{std})(T_{std}/T_a)]^{1/2}$	(°K = °C+273)	(mmHg)		
	Positive	Negative	ΔH_2O		(m ³ /min)	(ft ³ /min)					
5	1.9	1.8	3.7	1.90390	0.93791	32.0	31.27	305.0	760.0		
7	2.8	2.7	5.5	2.32025	1.13968	42.0	41.52	305.0	760.0		
10	4.0	3.9	7.9	2.77649	1.36078	52.0	51.40	305.0	760.0		
13	5.3	5.2	10.5	3.20602	1.56893	58.0	57.33	305.0	760.0		
18	6.4	6.3	12.7	3.52535	1.72368	62.0	61.28	305.0	760.0		

Linear Regression Y ON X : Y= mX + b


1	Slope (m)	2.0635	Linear Equation		Average	305.0	760.0		
2	Intercept(b)	-0.03151	Set Point Flow Rate (X) (m ³ /min)	1.133	r ²	0.982631	Pstd(mmHg)	760.0	
3	Correlation Coefficient (r)	0.99993	Final Set Flow Rate = (I)	0	r	0.99127746	T _{NTP}	298.0	
Result							(Pa/Pstd)*(Tstd/Ta)	0.97704918	
							C=(Pa/Pstd)*(Tstd/Ta)^0.5	0.988457981	

COMMENT

Andersen Instruments, Inc.

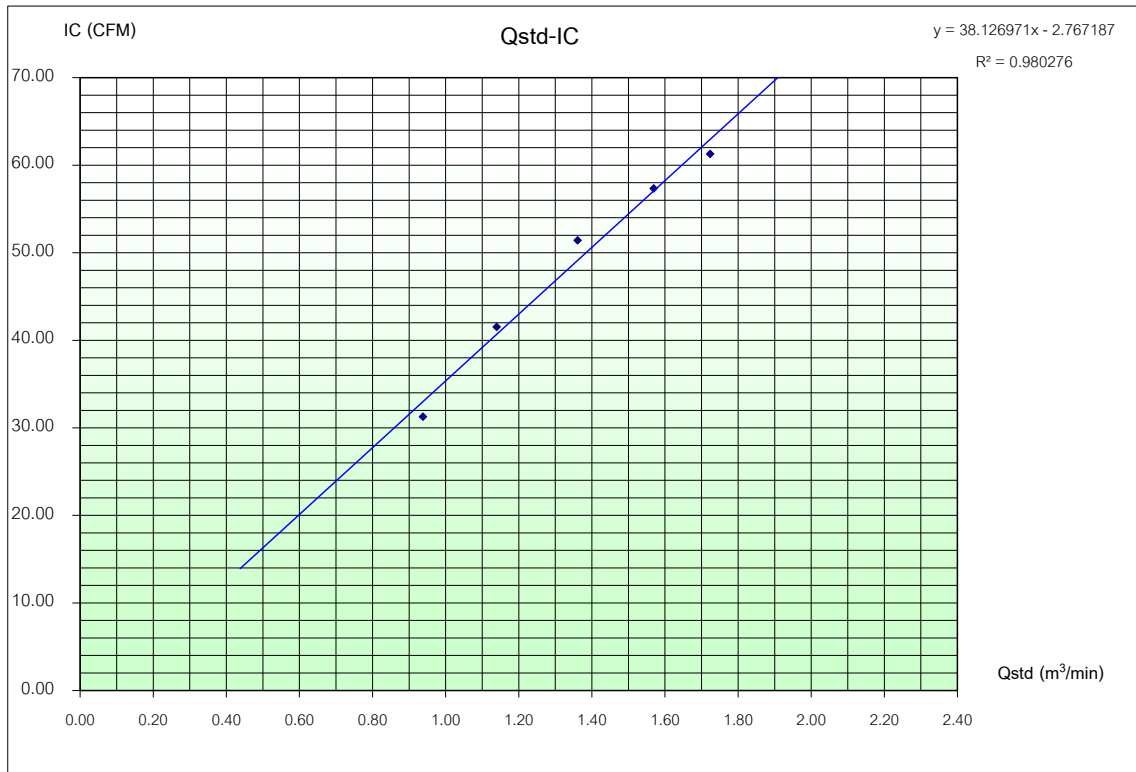

Calibrated By


Mr.Pasagorn Samol
Technician



บริษัท เอ็นไวร์ เซอร์วิส จำกัด
ENVIR SERVICE CO., LTD.

บริษัท เอ็นไวร์ เซอร์วิส จำกัด

42 รามอินทรา 14 แยก 9 แขวงท่าแร้ง เขตบางเขน กรุงเทพฯ 10230 โทรศัพท์ 02-9435814-5 โทรสาร 02-9438201

42 Raminthra 14 yeak 9, Tha Rang, Bangkhen, Bangkok 10230 Tel : 02-9435814-5 Fax : 02-9438201

Analyzer Performance Test

Calibrated Date: 22 April 2022

Instruments Information

Analyzer Type: CO Analyzer Model: 48C	Manufacturer Thermo Environmental S/N: 0604815182
------------------------------------------	------------------------------------------------------

Calibration System


Calibrator Unit	Standard Gas
Dilutor Model Dasibi Model 5008 S/N: 705 ZERO AIR Generator API MODEL 701 S/N: 1924	NO Conc 55.47 PPM SO2 Conc 55.11 PPM CO Conc 4,535 PPM Cylinder number EB0129027 Expire Date: 29 Oct. 2027

Environment: Temperature 25.5 °C

Humidity: 51 %RH

Calibration Report

Status	Zero			Span		
	Reference (PPM)	Reading (PPM)	Drift (PPM)	Reference (PPM)	Reading (PPM)	Drift%
Before	0.0	0.2	0.2	44.2	45.0	1.7
After	0.0	0.0	0.0	45.0	45.0	0.0

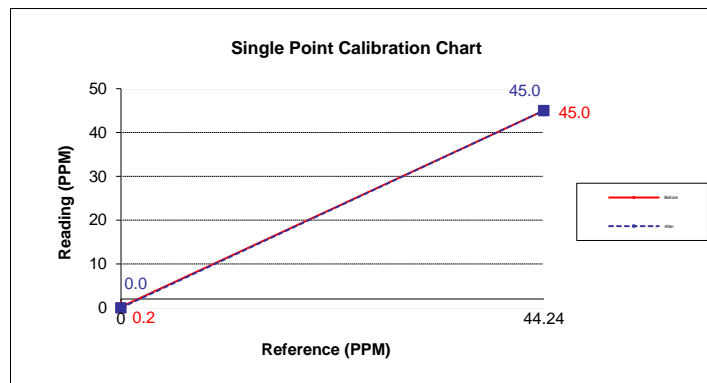

Calibrate By :

Mr. PASAGORN SAMOL

CERTIFICATE OF CALIBRATION

NO. 20241008092

Name of Product:	Sound Level Meter
Model:	ST-21D
Serial Number:	821086
Specification:	Class 2
Conclusion:	Pass
Date of calibration:	2025-02-24
Due Date:	2026-02-23

Calibrated by:




- This report certifies that all calibration equipment used in the test is traceable with the internal ISO9001 procedures and meets all specification given in the Manual(s) or respectively surpass then, and applies only to the unit identified above.
- This certificate is produced with advanced equipment & procedures which permit comprehensive quality assurance verification of all data supplied herein.
- This certificate of calibration shall not be reproduced except in full, without written permission of the Scarlet Tech Co Ltd Taiwan.

1. Preliminary inspection: OK

 2. Type & serial No. of Microphone: AWA14421A-000423

3. Adjustments to indicated sound levels:

 Type of Calibrator B&K 4231

 Sound Pressure Level 94.0 dB

 Equivalent Free-field Sound Level (reference environment conditions) 93.8 dB

 4. Measuring up limit: 138 dBA

5. Frequency weightings (Acoustic signal tests for Z weighting, other electric signal tests.)

Nominal frequency /Hz	Frequency weighting / dB			Nominal frequency /Hz	Frequency weighting / dB		
	A	C	Z		A	C	Z
20	-50.5	-6.3	-0.1	1000	0.0	0.0	0.0
31.5	-39.6	-3.1	0.0	2000	1.3	-0.2	0.0
63	-26.3	-0.8	-0.1	4000	1.2	-0.6	0.0
125	-16.2	-0.3	-0.1	8000	-1.2	-3.2	0.0
250	-8.7	-0.1	0.0	12500	-11.0	-13.0	0.0
500	-3.3	0.0	0.0	/	/	/	/

6. Self-generated noise

Microphone replaced by electrical input signal device

25.4 dB(A)	27.5 dB(C)	38.2 dB(Z)
------------	------------	------------

7. F&S Weighting

Rate of the F weighting decrease (dB/s)	35.3
Rate of the S weighting decrease (dB/s)	4.5
Deviation of F&S	0.0

8. Level Linearity (A-weighting at frequency 1 kHz)

Reference sound level 90.0 dB

Max error at 10dB steps upper reference sound level 0.1 dB

Max error at 1dB steps within 5dB of the upper limit linear operating range 0.0 dB

Max error at 10dB steps below reference sound level 0.1 dB

Max error at 1dB steps within 5dB upper the lower limit linear operating range 0.1 dB

9. Tone burst response (A Weighting) :

Single Toneburst duration /ms	Toneburst response /dB			
	L _{Afmax} -L _A	L _{ASmax} -L _A	L _{AE} -L _A	L _{AeqT} -L _A
500	0.0	-4.0	-2.9	-7.0
200	-1.0	7.4	-6.9	-7.0
2	-18.0	-27.0	-27.0	-7.0
0.25	-27.2	/	-36.1	-7.0

10. Peak C sound level (500Hz) :

Cycle	One cycle	nominal value	Positive half	nominal value	Negative half	nominal value
LC _{peak} -LC(dB)	3.5	3.5	2.4	2.4	2.4	2.4

11. Overload indication: Pass

12. Statistical analysis function

Sweep signal maximum indicated sound level: 123.0 dB

Sweep amplitude: 40 dB

Scan cycle time: 60 S; Measurement period: 180 S.

Items	Measured value/dB	Theoretical calculated value/dB	Error/dB
L _{Aeq,T}	113.3	113.4	-0.1
L ₅	121.0	121.0	0.0
L ₁₀	119.0	119.0	0.0
L ₅₀	103.0	103.0	0.0
L ₉₀	87.1	87.0	0.1
L ₉₅	85.1	85.0	0.1

Uncertainty of measurement results: 0.4 dB (k=2)

Environment conditions:

Air temperature: 25 °C

Relative humidity: 65 %

Static pressure: 100.0 kPa

References:

IEC 61672-3 Sound Level Meters Part 3: Periodic tests

Calibration Certificate

Part Number: 721A2601

Description: Micromate with DIN Geophone

Serial Number: UM16257

Calibration Date: NOV 30 2021

Calibration Reference Equipment: 714J7402

Instantel certifies that the above product was calibrated in accordance with the applicable Instantel procedures. These procedures are part of a quality system that is designed to assure that the product listed above meets or exceeds Instantel specifications.

Instantel further certifies that the measurement instruments used during the calibration of this product are traceable to the National Institute of Standards and Technology; or National Research Council of Canada. Evidence of traceability is on file at Instantel and is available upon request.

The environment in which this product was calibrated is maintained within the operating specifications of the instrument.

Please note that the sensor check function is intended to check that the sensors are connected to the unit, installed in the proper orientation and sufficiently level to operate properly. This function should not be confused with a formal calibration, which requires the sensors be checked against a reference that is traceable to a known standard. Instantel recommends that products be returned to Instantel or an authorized service and calibration facility for annual calibration.

Calibrated By: _____




Xiaoming Yang



Instantel®

309 Legget Drive, Ottawa, Ontario, K2K 3A3, (613) 592-4642

Frequency Response of UM16257

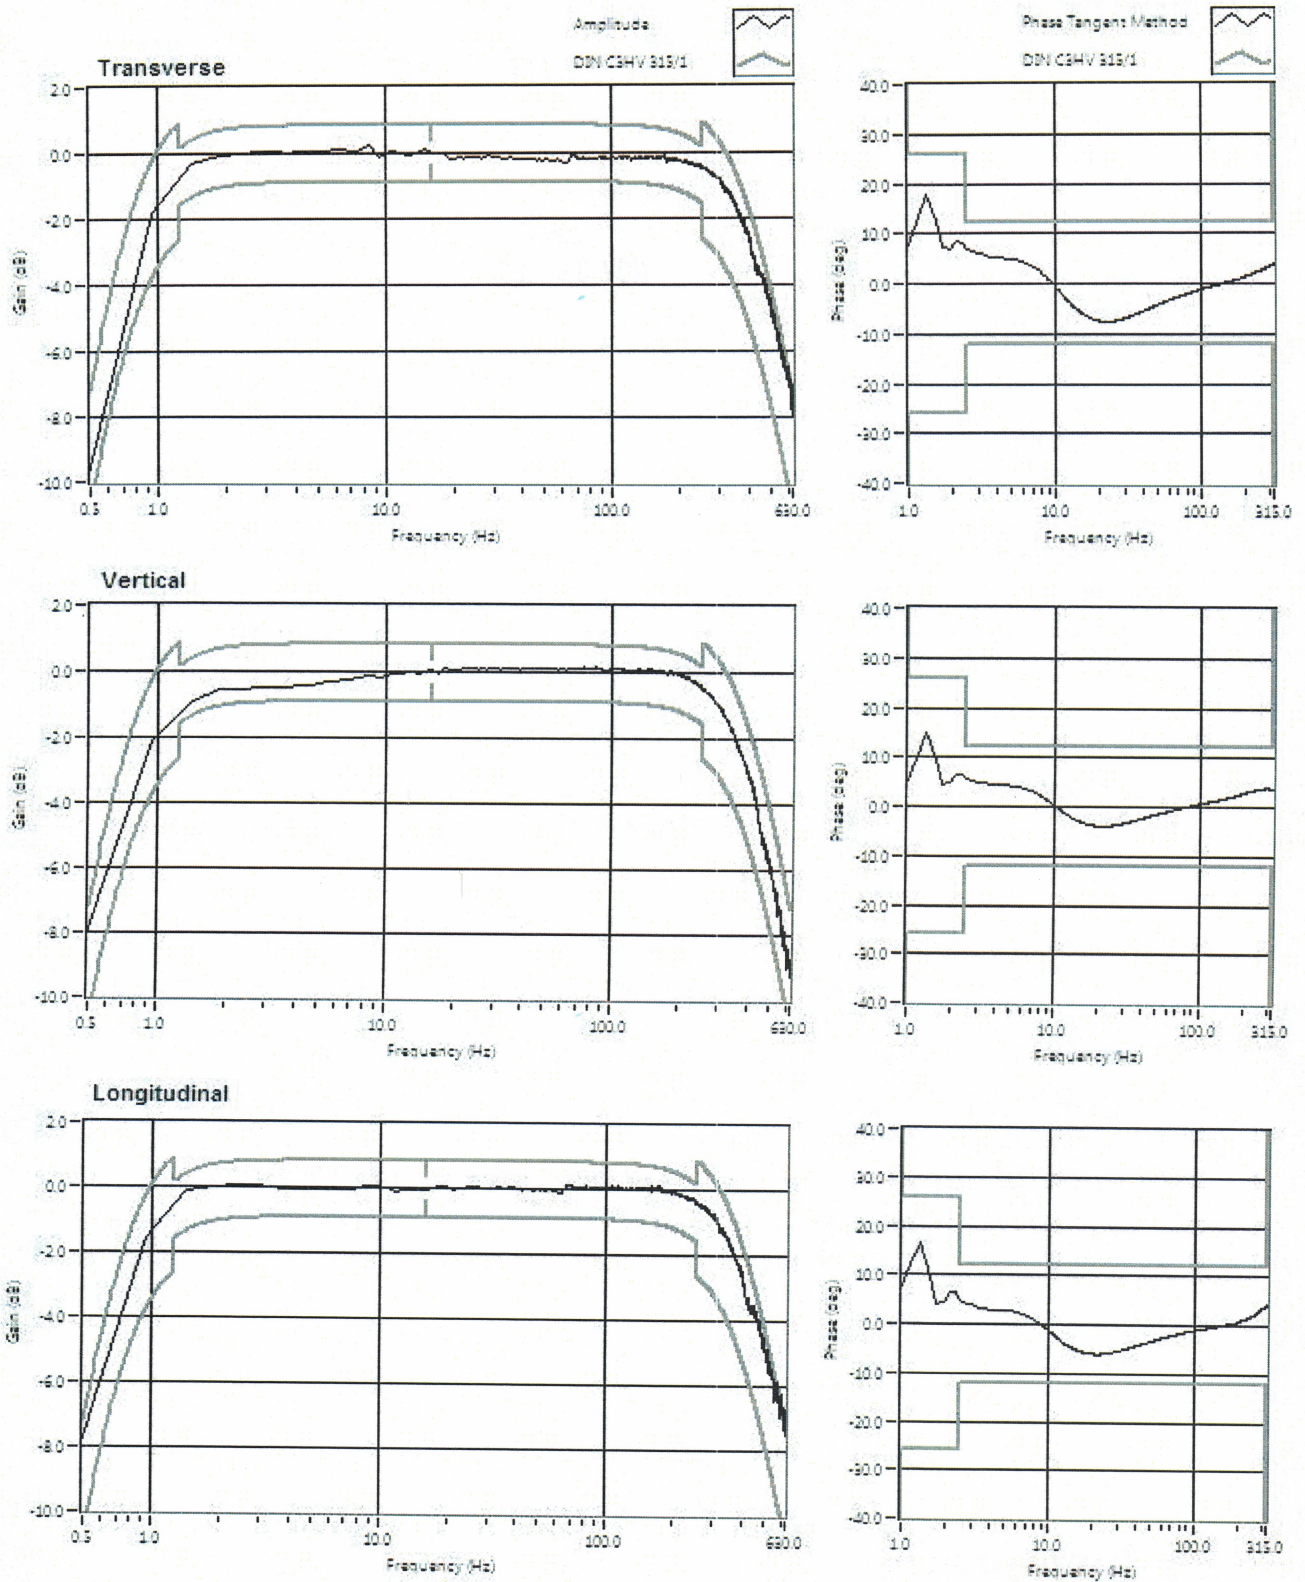



สภาวិศวกกร

ตามพระราชบัญญัติวิศวกกร พ.ศ. ๒๕๕๒
ออกใบอนุญาตนี้ให้ไว้เพื่อแสดงว่า

บริษัท กรีน เอ็นไว เอ็นจิเนียริง จำกัด
ได้รับอนุญาตประกอบวิชาชีพวิศวกรรมควบคุม
เลขทะเบียน ๑๕๖๕/๖๒

ตั้งแต่วันที่ ๑๖ สิงหาคม ๒๕๖๗ ถึงวันที่ ๑๕ สิงหาคม ๒๕๗๐

นายชเนต วิระศิริ

(นายชเนต วิระศิริ)
นายกสภาวิศวกกร