ภาคผนวก ง

เอกสารสอบเทียบเครื่องมือที่ใช้ในการวิเคราะห์

right solutions.
right partner.

รายการเครื่องมือที่ใช้ในการวิเคราะห์ / ทดสอบ

Sample Name	Parameter	Equipment Name	ID No.	Calibrated Date	Next Cal	Freq. Calibrate (Months)
Ambient	Total Suspended Particulate	High Volume	RYG_FS0663	-	-	On site Calibration
Ambient	Total Suspended Particulate	High Volume	RYG_FS0177	-	-	On site Calibration
Ambient	Total Suspended Particulate	High Volume	RYG_FS0176	-	-	On site Calibration
Ambient	Total Suspended Particulate	Digital Balance	RYG_EN0001	20-Feb-25	20-Feb-26	12
Ambient	Nitrogen Dioxide	NO_2 Analyzer	RYG_FS0453	3-Jul-25	3-Jan-26	6
Ambient	Nitrogen Dioxide	NO_2 Analyzer	RYG_FS0272	2-Jul-25	2-Jan-26	6
Ambient	Nitrogen Dioxide	NO_2 Analyzer	RYG_FS0457	3-Jul-25	3-Jan-26	6
Ambient	Wind Speed / Wind Direction	Wind Speed / Wind Direction	RYG_FS0413	29-Oct-24	29-Apr-26	18
Ambient	Wind Speed / Wind Direction	Wind Speed / Wind Direction	RYG_FS0089	7-Oct-24	7-Apr-26	18
Ambient	Wind Speed / Wind Direction	Wind Speed / Wind Direction	RYG_FS0414	29-Oct-24	29-Apr-26	18
Stack	Carbon Monoxide	Console Control Unit	BKK_FS0468	10-Jul-25	10-Jan-26	6
Stack	Carbon Monoxide	Pitot Tube	BKK_FS0472	10-Jul-25	10-Jan-26	6
Stack	Carbon Monoxide	Fuel Gas Analyzer	RYG_FS0464	24-Mar-25	23-Mar-26	12
Stack	Carbon Monoxide	DRYCAL FLOWMETER	RYG_FS0208	27-Jan-25	26-Jan-26	12
Stack	Carbon Monoxide	DRYCAL FLOWMETER	BKK_FS0614	9-Sep-24	9-Sep-25	12
Stack	Carbon Monoxide	Air Sampling Pump	RYG_FS0144	7-Jul-25	7-Oct-25	3
Stack	Carbon Monoxide	CO Analyzer	RYG_EN0034	3-Jul-25	3-Jul-26	12
Stack	Oxides of Nitrogen	Console Control Unit	BKK_FS0468	10-Jul-25	10-Jan-26	6
Stack	Oxides of Nitrogen	Pitot Tube	BKK_FS0472	10-Jul-25	10-Jan-26	6
Stack	Oxides of Nitrogen	Fuel Gas Analyzer	RYG_FS0464	24-Mar-25	23-Mar-26	12
Stack	Oxides of Nitrogen	Vacuum Gauge	RYG_FS0333	3-Oct-24	2-Apr-26	18
Stack	Oxides of Nitrogen	SPECTROPHOTOMETER	RYG_EN0037	18-Mar-25	18-Sep-26	18
Stack	Total Suspended Particulate	Console Control Unit	BKK_FS0468	10-Jul-25	10-Jan-26	6
Stack	Total Suspended Particulate	Pitot Tube	BKK_FS0472	10-Jul-25	10-Jan-26	6
Stack	Total Suspended Particulate	Fuel Gas Analyzer	RYG_FS0464	24-Mar-25	23-Mar-26	12
Stack	Total Suspended Particulate	Digital Balance	RYG_EN0003	20-Feb-25	20-Feb-26	12
Workplace	Total Dust	DRYCAL FLOWMETER	RYG_FS0208	27-Jan-25	26-Jan-26	12
Workplace	Total Dust	DRYCAL FLOWMETER	BKK_FS0614	9-Sep-24	9-Sep-25	12
Workplace	Total Dust	DRYCAL FLOWMETER	BKK_FS0614	10-Sep-25	9-Sep-26	12
Workplace	Total Dust	DRYCAL FLOWMETER	BKK_FS0619	9-Sep-24	9-Sep-25	12
Workplace	Total Dust	DRYCAL FLOWMETER	BKK_FS0619	10-Sep-25	9-Sep-26	12
Workplace	Total Dust	Digital Balance	RYG_EN0004	20-Feb-25	20-Feb-26	12
Workplace	Styrene	DRYCAL FLOWMETER	RYG_FS0208	27-Jan-25	26-Jan-26	12
Workplace	Styrene	DRYCAL FLOWMETER	BKK_FS0614	9-Sep-24	9-Sep-25	12
Workplace	Styrene	DRYCAL FLOWMETER	BKK_FS0614	10-Sep-25	9-Sep-26	12
Workplace	Styrene	DRYCAL FLOWMETER	BKK_FS0619	9-Sep-24	9-Sep-25	12
Workplace	Styrene	DRYCAL FLOWMETER	BKK_FS0619	10-Sep-25	9-Sep-26	12
Workplace	Styrene	GC-MSD	BKK_EN0049	25-Oct-24	25-Apr-26	18
Workplace	Total Hydrocarbon	DRYCAL FLOWMETER	RYG_FS0208	27-Jan-25	26-Jan-26	12
Workplace	Total Hydrocarbon	DRYCAL FLOWMETER	BKK_FS0614	9-Sep-24	9-Sep-25	12
Workplace	Total Hydrocarbon	DRYCAL FLOWMETER	BKK_FS0614	10-Sep-25	9-Sep-26	12
Workplace	Total Hydrocarbon	DRYCAL FLOWMETER	BKK_FS0619	9-Sep-24	9-Sep-25	12
Workplace	Total Hydrocarbon	DRYCAL FLOWMETER	BKK_FS0619	10-Sep-25	9-Sep-26	12
Workplace	Total Hydrocarbon	Total Hydrocarbon Analyzer	RYG_EN0038	6-Mar-25	6-Mar-26	12
Noise	Leq 24 hrs	Sound Calibrator	RYG_FS0213	16-Jan-25	16-Jan-26	12
Noise	Leq 24 hrs	Sound Level Meter	RYG_FS0381	9-Oct-24	9-Oct-25	12
Noise	Leq 24 hrs	Sound Level Meter	RYG_FS0384	9-Oct-24	9-Oct-25	12
Noise	Leq 24 hrs	Sound Level Meter	RYG_FS0386	9-Oct-24	9-Oct-25	12
Noise	Leq 8 hrs	Sound Calibrator	RYG_FS0213	16-Jan-25	16-Jan-26	12
Noise	Leq 8 hrs	Sound Level Meter	RYG_FS0301	27-Jan-25	26-Jan-26	12
Noise	Leq 8 hrs	Sound Level Meter	RYG_FS0432	27-Jan-25	26-Jan-26	12
Noise	Leq 8 hrs	Sound Level Meter	RYG_FS0433	27-Jan-25	26-Jan-26	12
Noise	Leq 8 hrs	Sound Level Meter	RYG_FS0434	27-Jan-25	26-Jan-26	12
Noise	Leq 8 hrs	Sound Calibrator	RYG_FS0496	19-Mar-25	19-Mar-26	12
Noise	Leq 8 hrs	Sound Level Meter	RYG_FS0018	21-Jan-25	21-Jan-26	12
Noise	Leq 8 hrs	Sound Level Meter	RYG_FS0019	21-Jan-25	21-Jan-26	12
Noise	Leq 8 hrs	Sound Level Meter	RYG_FS0022	19-Mar-25	19-Mar-26	12
Noise	Leq 8 hrs	Sound Level Meter	RYG_FS0431	27-Jan-25	26-Jan-26	12

right solutions.
right partner.

รายการเครื่องมือที่ใช้ในการวิเคราะห์ / ทดสอบ

Sample Name	Parameter	Equipment Name	ID No.	Calibrated Date	Next Cal	Freq. Calibrate (Months)
Rayong Lab	pH at 25 °C	pH Meter	RYG_EN0183	18-Jul-25	18-Jan-27	18
Rayong Lab	BOD	DO meter with Sensor	RYG_EN0032	20-Jan-25	20-Jul-26	18
Rayong Lab	BOD	Incubator	RYG_EN0154	1-Nov-24	1-May-26	18
Rayong Lab	BOD	Burette	RYG_EN0216	18-Sep-25	18-Sep-26	12
Rayong Lab	COD	Spectrophotometer	RYG_EN0037	18-Mar-25	18-Sep-26	18
Rayong Lab	Total Suspended Solids	Electronic Balance	RYG_EN0163	20-Feb-25	20-Feb-26	12
Rayong Lab	Total Suspended Solids	Chamber (Oven)	RYG_EN0012	10-Sep-25	10-Mar-27	18
Rayong Lab	Total Dissolved Solids 180°C	Electronic Balance	RYG_EN0163	20-Feb-25	20-Feb-26	12
Rayong Lab	Total Dissolved Solids 180°C	Chamber (Oven)	RYG_EN0012	10-Sep-25	10-Mar-27	18
Rayong Lab	Total Kjeldahl Nitrogen	Block Digestion Unit	RYG_EN0188	10-Sep-25	10-Mar-27	18
Rayong Lab	Total Kjeldahl Nitrogen	pH Meter	RYG_EN0183	18-Jul-25	18-Jan-27	18
Rayong Lab	Oil & Grease	Electronic Balance	RYG_EN0003	20-Feb-25	20-Feb-26	12
Rayong Lab	Oil & Grease	Liquid Bath (Water)	RYG_EN0220	27-Nov-25	27-Nov-26	12
Rayong Lab	Temperature	pH meter	RYG_FS0596	25-Jun-25	25-Jun-26	12
Rayong Lab	Color (at Original pH)	Spectrophotometer	RYG_EN0037	18-Mar-25	18-Sep-26	18
Rayong Lab	Color (at pH 7.0)	Spectrophotometer	RYG_EN0037	18-Mar-25	18-Sep-26	18
Rayong Lab	Cyanide	SPECTROPHOTOMETER	RYG_EN0037	18-Mar-25	18-Sep-26	18
Rayong Lab	Formaldehyde	SPECTROPHOTOMETER	RYG_EN0037	18-Mar-25	18-Sep-26	18
Rayong Lab	Phenol	SPECTROPHOTOMETER	RYG_EN0037	18-Mar-25	18-Sep-26	18
Rayong Lab	Sulfide	Chamber (Cold Room)	RYG_EN0184	27-Nov-25	27-May-27	18
Rayong Lab	Residual Free Chlorine	Chamber (Cold Room)	RYG_EN0184	27-Nov-25	27-May-27	18
Rayong Lab	Conductivity	Conductivity meter	RYG_EN0200	21-Mar-25	21-Mar-26	12
Rayong Lab	Total Petroleum Hydrocarbon	Electronic Balance	RYG_EN0003	20-Feb-25	20-Feb-26	12
Rayong Lab	Total Petroleum Hydrocarbon	Liquid Bath (Water)	RYG_EN0220	27-Nov-25	27-Nov-26	12
Water Lab	Hexavalent Chromium	Spectrophotometer	BKK_EN0356	8-Oct-25	8-Oct-26	12
Water Lab	Barium	ICP-MS	BKK_EL0043	4-Oct-24	3-Apr-26	18
Water Lab	Barium	Hot Block	BKK_EL0054	4-Mar-25	4-Sep-26	18
Water Lab	Barium	Chamber (Cooling Room)	BKK_EN0167	4-Jun-25	4-Dec-26	18
Water Lab	Lead	ICP-MS	BKK_EL0043	4-Oct-24	3-Apr-26	18
Water Lab	Lead	Hot Block	BKK_EL0054	4-Mar-25	4-Sep-26	18
Water Lab	Lead	Chamber (Cooling Room)	BKK_EN0167	4-Jun-25	4-Dec-26	18
Water Lab	Manganese	ICP-MS	BKK_EL0043	4-Oct-24	3-Apr-26	18
Water Lab	Manganese	Hot Block	BKK_EL0054	4-Mar-25	4-Sep-26	18
Water Lab	Manganese	Chamber (Cooling Room)	BKK_EN0167	4-Jun-25	4-Dec-26	18
Water Lab	Nickel	ICP-MS	BKK_EL0043	4-Oct-24	3-Apr-26	18
Water Lab	Nickel	Hot Block	BKK_EL0054	4-Mar-25	4-Sep-26	18
Water Lab	Nickel	Chamber (Cooling Room)	BKK_EN0167	4-Jun-25	4-Dec-26	18
Water Lab	Arsenic	ICP-MS	BKK_EL0043	4-Oct-24	3-Apr-26	18
Water Lab	Arsenic	Hot Block	BKK_EL0054	4-Mar-25	4-Sep-26	18
Water Lab	Arsenic	Chamber (Cooling Room)	BKK_EN0167	4-Jun-25	4-Dec-26	18
Water Lab	Selenium	ICP-MS	BKK_EL0043	4-Oct-24	3-Apr-26	18
Water Lab	Selenium	Hot Block	BKK_EL0054	4-Mar-25	4-Sep-26	18
Water Lab	Selenium	Chamber (Cooling Room)	BKK_EN0167	4-Jun-25	4-Dec-26	18
Water Lab	Cadmium	ICP-MS	BKK_EL0043	4-Oct-24	3-Apr-26	18
Water Lab	Cadmium	Hot Block	BKK_EL0054	4-Mar-25	4-Sep-26	18
Water Lab	Cadmium	Chamber (Cooling Room)	BKK_EN0167	4-Jun-25	4-Dec-26	18
Water Lab	Trivalent Chromium	ICP-MS	BKK_EL0043	4-Oct-24	3-Apr-26	18
Water Lab	Trivalent Chromium	Hot Block	BKK_EL0054	4-Mar-25	4-Sep-26	18
Water Lab	Trivalent Chromium	Chamber (Cooling Room)	BKK_EN0167	4-Jun-25	4-Dec-26	18
Water Lab	Mercury	DUO-CVAFS / CVAAS	BKK_EL0023	12-Dec-24	12-Jun-26	18
Water Lab	Copper	ICP-MS	BKK_EL0043	4-Oct-24	3-Apr-26	18
Water Lab	Copper	Hot Block	BKK_EL0054	4-Mar-25	4-Sep-26	18
Water Lab	Copper	Chamber (Cooling Room)	BKK_EN0167	4-Jun-25	4-Dec-26	18
Water Lab	Zinc	ICP-MS	BKK_EL0043	4-Oct-24	3-Apr-26	18
Water Lab	Zinc	Hot Block	BKK_EL0054	4-Mar-25	4-Sep-26	18
Water Lab	Zinc	Chamber (Cooling Room)	BKK_EN0167	4-Jun-25	4-Dec-26	18
Water Lab	Total Organic carbon	TOC Analyzer	BKK_EN0066	27-Jun-25	27-Jun-26	12
Water Lab	Organochlorine Pesticide	GC MSMS	BKK_EN0284	21-Nov-24	21-May-26	18

High Volume Air Sampler Calibration Worksheet

Project Site :	Siam Polystyrene Co., Ltd.	**Barometric Pressure (mm Hg) :**	756.3
Calibrate Location :	ริมรั้วด้านทิศตะวันตกของ บริษัท ปุ๋ยเอ็น เอฟซี จำกัด (มหาชน)	**Temperature (°C) :**	29.7
Calibrate Date :	22-Sep-25	**High Volume ID :**	RYG_FS0663
CalibrationSheet No.:	**C-220925-RYG_FS0663**	**High Volume Model :**	TE-5009X
Calibrator ID:	RYG_FS0205	**High Volume S/N :**	6260
Calibrator Model :	TE-5028A	**Calibrator Slope :**	1.52567
Calibrator S/N :	1166	**Calibrator Intercept :**	-0.03613

Test No.	Delta H_2O (inch)	Q_{std} (m^3/min)	I : Chart (CFM)	Linear Regression
1	2.7	1.1021	40	Slope : 32.5925
2	3.7	1.2840	46	Intercept : 4.1867
3	4.4	1.3970	50	Correlation Coefficient : 0.9998
4	5.3	1.5297	54	
5	6.7	1.7154	60	

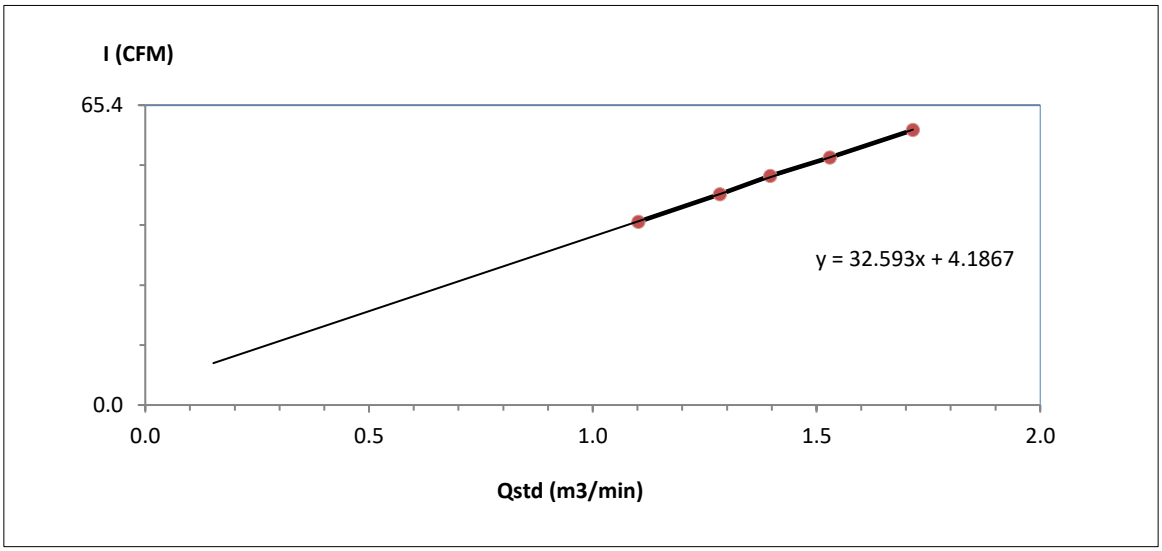

Calibrated by _____

(Mr. Nontachai Uppathame)
RYG Field Services Scientist (2)

Approved by : _____

(Mr. Supot Salamteh)
Field Services Section Head

High Volume Air Sampler Calibration Worksheet

Project Site :	Siam Styrene Monomer Co., Ltd	**Barometric Pressure (mm Hg) :**	756.3
Calibrate Location :	บ้านอ่าวประดู่ (โรงพยาบาลส่งเสริมสุขภาพตำบลตากวน)	**Temperature (°C) :**	29.7
Calibrate Date :	22-Sep-25	**High Volume ID :**	RYG_FS0177
CalibrationSheet No.:	**C-220925-RYG_FS0177**	**High Volume Model :**	TE-5170D
Calibrator ID:	RYG_FS0205	**High Volume S/N :**	4803
Calibrator Model :	TE-5028A	**Calibrator Slope :**	1.52567
Calibrator S/N :	1166	**Calibrator Intercept :**	-0.03613

Test No.	Delta H_2O (inch)	Q_{std} (m^3/min)	I : Chart (CFM)	Linear Regression
1	2.8	1.1217	40	Slope : 32.9827
2	3.8	1.3008	46	Intercept : 3.0221
3	4.6	1.4275	50	Correlation Coefficient : 1.0000
4	5.4	1.5437	54	
5	6.8	1.7279	60	

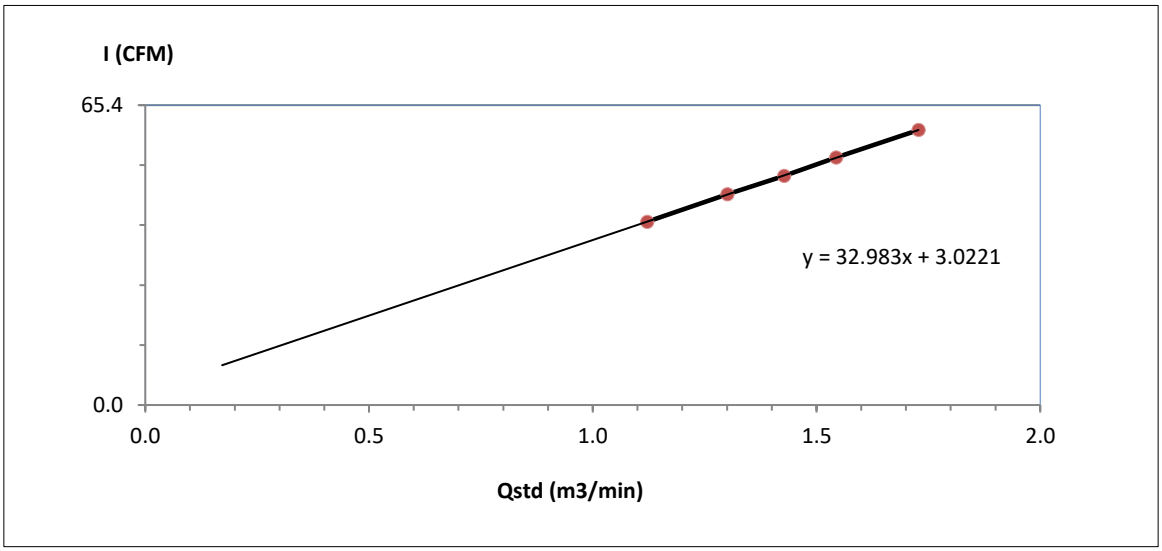

Calibrated by _____

(Mr. Nontachai Uppathame)
RYG Field Services Scientist (2)

Approved by : _____

(Mr. Supot Salamteh)
Field Services Section Head

High Volume Air Sampler Calibration Worksheet

Project Site :	Siam Styrene Monomer Co., Ltd	**Barometric Pressure (mm Hg) :**	756.3
Calibrate Location :	บ้านมาบตาพุด	**Temperature (°C) :**	29.7
Calibrate Date :	22-Sep-25	**High Volume ID :**	RYG_FS0176
CalibrationSheet No.:	**C-220925-RYG_FS0176**	**High Volume Model :**	TE-5170D
Calibrator ID:	RYG_FS0205	**High Volume S/N :**	4802
Calibrator Model :	TE-5028A	**Calibrator Slope :**	1.52567
Calibrator S/N :	1166	**Calibrator Intercept :**	-0.03613

Test No.	Delta H_2O (inch)	Q_{std} (m^3/min)	I : Chart (CFM)	Linear Regression
1	2.6	1.0822	40	Slope : 31.4216
2	3.6	1.2671	46	Intercept : 6.0645
3	4.4	1.3970	50	Correlation Coefficient : 0.9999
4	5.3	1.5297	54	
5	6.7	1.7154	60	

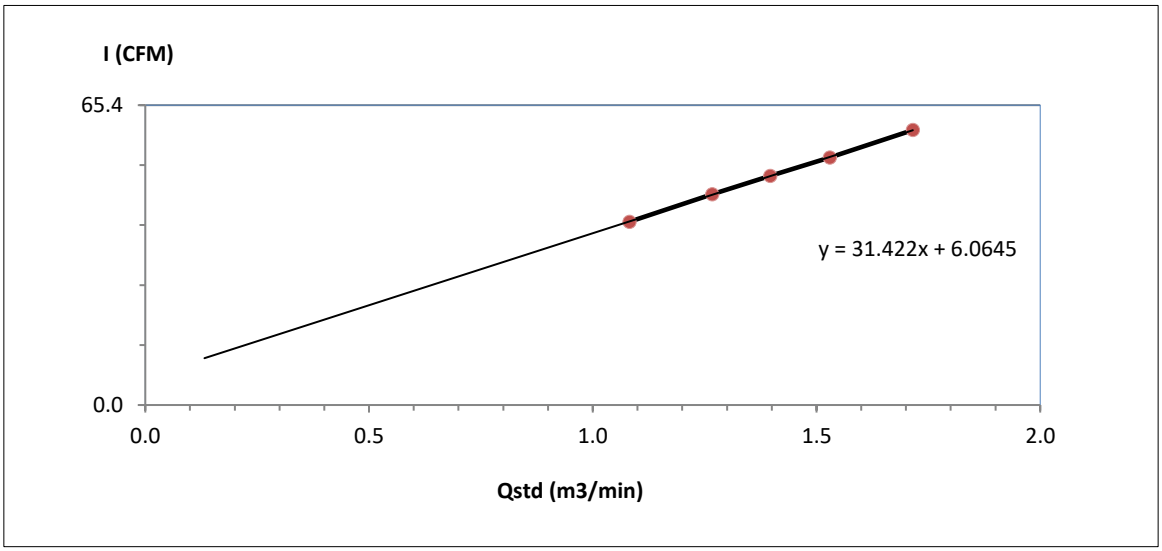

Calibrated by _____

(Mr. Nontachai Uppathame)
RYG Field Services Scientist (2)

Approved by : _____

(Mr. Supot Salamteh)
Field Services Section Head

Accredited by

NSC-TISI-TIS 17025
Calibration 0426

Calibration certificate

Calibration Certificate No. 25BKL0001

Object	Electronic non-automatic weighing instrument
Manufacturer	Sartorius
Type	LA130S-F
Serial | QM Ident. no.	25409664 | RYG_EN0001
Customer	ALS Laboratory Group (Thailand) Co.,Ltd. (Rayong Branch) 616/10 Moo 5 T.Maenam Khu, A.Pluak Daeng, Rayong 21140, Thailand.
Order no.	2230
Number of pages	4
Date of calibration	20 Feb 2025

This calibration certificate documents the traceability to national standards.

Uncertainties of measurements are taken into account when only statements of compliance are made.

This certificate was prepared by Sartorius Corporation in accordance to the current ISO/IEC 17025:2017 standard and Sartorius Work Instruction (Method) SOP WI 08.

This certificate relate and apply this equipment only.

REVIEW BY ..... Thanitak.

APPROVED BY..... D.Thanon.

NEXT CAL DATE..... 20/02/26

This calibration certificate may not be reproduced other than in full except with the permission of NSC-TISI-TIS-17025 and the issuing laboratory. Calibration certificates without signature are not valid.

The user is obliged to have the object recalibrated at appropriate intervals.

Date	Approval of the Calibration Certificate	Person in charge
06 Mar 2025	Mr. Chonchai Inthana	Kachen Lalee

Calibration object

Single range instrument

Model	LA130S-F
Serial Number	25409664
QM Ident. no | Inventory no.	RYG_EN0001 | ---

Maximum capacity (Max. load)	150.0000 g
Measured range	150.0000 g
Scale interval	0.0001 g

Place of calibration

Address	According to page 1
Department | Cost center	Laboratory Department. | ---
Building | Floor	--- | 1st Floor.
Room	Balance Room.
Maximum temperature variation at place of calibration	5 K

Calibration procedure

EURAMET cg-18, V4.0 - Guidelines on the Calibration of Non-Automatic Weighing Instruments

Test equipment

Test equipment type	Test equipment ID	Valid until
Thermometer	MHB-382SD s/nB011342 Traceable to SI unit through DKSH	21 Aug 2025
Test weight set OIML R111 E2	Certificate No.M2308197S ,E2(Traceable to SI unit through TCS)	23 Aug 2025

Adjustment Status

The measuring device was internally adjusted before the calibration.

Environmental and measuring conditions

Date of calibration	20 Feb 2025
Temperature at place of calibration | Temp. diff. $T_{weights}$ - T_{place}	24.5 °C | 1.0 K
Measuring conditions	The installation site is suitable. The device was levelled. Balance was loaded up to Max before test.
Comments	Humidity 58.0 %RH.

Measurement results | Measurement uncertainties

Repeatability

Test load (nominal): 10 g | 100 g

	10 g	100 g
1	10.0000 g	100.0000 g
2	9.9999 g	100.0000 g
3	10.0000 g	99.9999 g
4	10.0000 g	100.0000 g
5	10.0000 g	99.9999 g
6	9.9999 g	99.9999 g
7	10.0000 g	100.0000 g
8	10.0000 g	100.0000 g
9	10.0000 g	100.0000 g
10	10.0000 g	100.0000 g
	s = 0.00004 g	s = 0.00005 g

Eccentricity

Test load (nominal):	**50 g**
Center	50.0000 g
Front left	50.0001 g
Back left	50.0000 g
Back right	49.9999 g
Front right	50.0001 g
Maximum deviation from centric loading indication $\lvert\Delta I_{ecc}\rvert_{max}$ = 0.0001 g	

Error of indication

Testload *L*	Indication *I*	Error *E*	Expansion factor *k*	Uncertainty *U*(*E*)	Uncertainty relative $U_{rel}(E)$
0.0100 g	0.0100 g	0.0000 g	2.00	0.00012 g	1.2 %
0.0500 g	0.0500 g	0.0000 g	2.00	0.00013 g	0.25 %
0.1000 g	0.1000 g	0.0000 g	2.00	0.00013 g	0.13 %
0.5000 g	0.5000 g	0.0000 g	2.00	0.00013 g	0.026 %
1.0000 g	1.0000 g	0.0000 g	2.00	0.00013 g	0.013 %
2.0000 g	2.0000 g	0.0000 g	2.00	0.00013 g	0.0065 %
5.0000 g	5.0000 g	0.0000 g	2.00	0.00013 g	0.0026 %
10.0000 g	10.0000 g	0.0000 g	2.00	0.00013 g	0.0013 %
20.0000 g	20.0000 g	0.0000 g	2.00	0.00014 g	0.00069 %
100.0000 g	100.0000 g	0.0000 g	2.00	0.00021 g	0.00021 %
150.0000 g	149.9999 g	-0.0001 g	2.00	0.00028 g	0.00019 %
Maximum error of indication		$\lvert E\rvert_{max}$ = 0.0001 g			

$U_{rel}(E)$ is the quotient of $U(E)$ and test load L. The uncertainty of measurement $U(E)$ is valid only if error E is considered. You will find reference notes on the uncertainty of measurement in use under: Appendix to the calibration certificate | Interpretation of measurement results.
Reference note: The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the documented Expansion factor, determined in accordance with the European Calibration Guideline EURAMET cg-18, V4.0. There is a 95 % probability that the value of the measurand will be in the assigned value range.

End of calibration certificate

Uncertainty of measurement in use

Device adjusted before measurement	Yes
Temperature deviation considered	1.5 K (isoCAL active)
Temperature coefficient considered	$1 \cdot 10^{-6}$/K
Uncertainty of the weighing result $U_{gl}(W)$	**$U_{gl}(W) = 0.00013\ g + 3.96 \cdot 10^{-6} \cdot R$**

Reference note: The current uncertainty of measurement is calculated by entering of the reading *R* into this formula. In relation to this, there is no need for a correction of the indication error. The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied with an Expansion factor of 2, determined in accordance with the European Calibration Guideline EURAMET cg-18, V4.0. There is a 95 % probability that the value of the measurand will be in the assigned value range.

Indication in % from max load	Net indication *R*	Uncertainty $U_{gl}(W)$	Uncertainty relative $U_{gl}(W)_{rel}$
1 %	1.5000 g	0.00014 g	0.0091 %
25 %	37.5000 g	0.00028 g	0.00074 %
50 %	75.0000 g	0.00043 g	0.00057 %
75 %	112.5000 g	0.00058 g	0.00051 %
100 %	150.0000 g	0.00072 g	0.00048 %

Graphic realization of the relative uncertainty of measurement | process accuracy

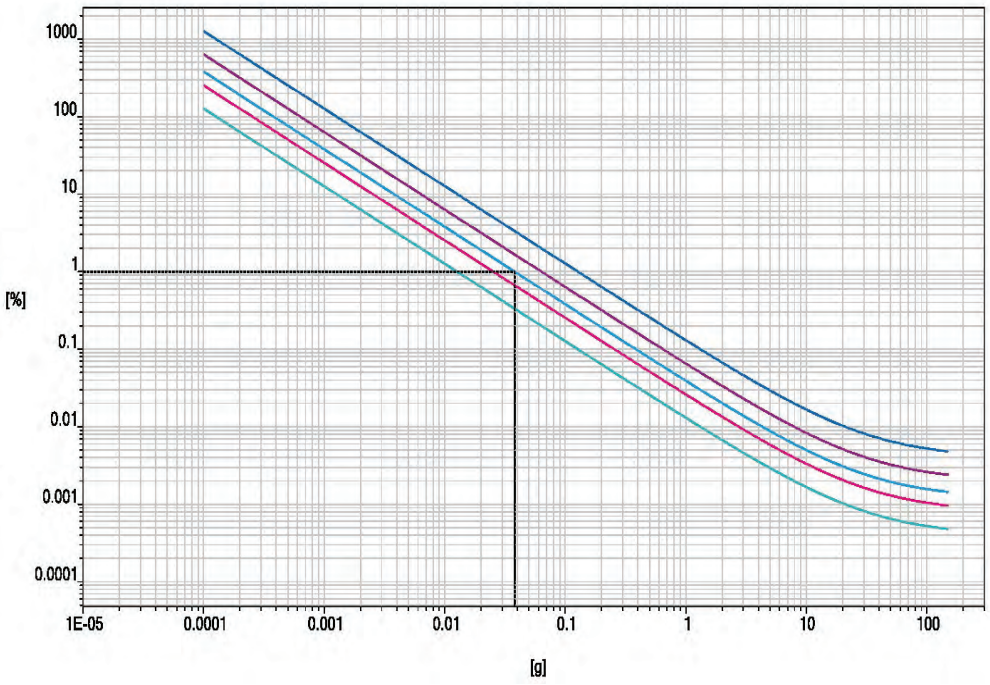



Displayed example

Process accuracy	1.00 %
Safety factor	3
Minimum sample weight	0.0380 g

MULTIPOINT CALIBRATION REPORT

Calibration Date	3-Jul-25	Equipment Name	NOx Analyzer
Manufacturer	HORIBA	Model	APNA-370
Serial No.	AWXG87CR	Equipment ID	RYG_FS0453
Calibrator Manufacturer	Teledyne API	Model	700
Serial No.	947		
Std. Gas Concentration (PPM)	55.88	Cylinder No.	GN0027222
Cylinder Pressure (psi)	1800	Certified By	Airgas Inc.
Certified Date	9-Feb-22	Expired Date	9-Feb-30

Point	CALIBRATION RESULTS						
	Ideal	Actual NO	Error NO	%Error NO	Actual NOx	Error NOx	%Error NOx
ZERO	0.00	0.10	0.10	0.10	0.10	0.10	0.10
1	100.00	99.60	-0.40	-0.40	101.10	1.10	1.10
2	200.00	198.60	-1.40	-0.70	199.70	-0.30	-0.15
3	300.00	299.00	-1.00	-0.33	298.60	-1.40	-0.47
4	400.00	401.20	1.20	0.30	401.10	1.10	0.28
AVERAGE (%)				-0.21			0.17

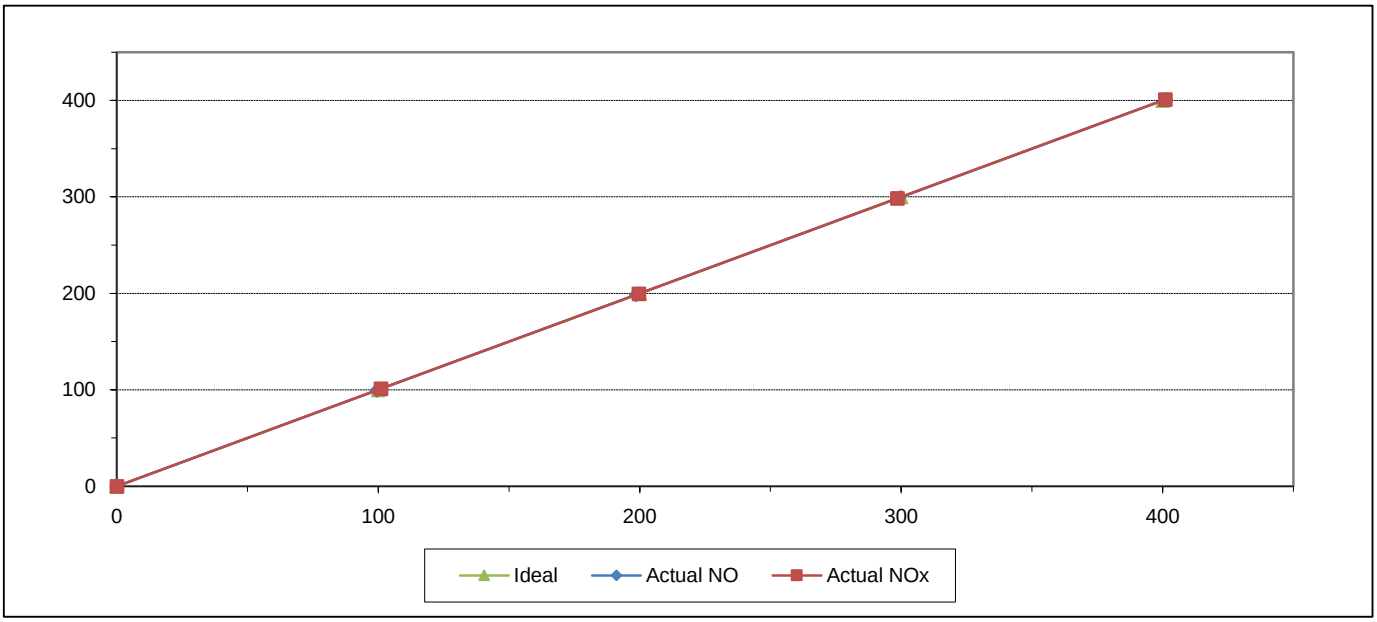

Calibrated By

(Mr.Jirawut Sakarn)
Field Environmental Scientist (3)

Approved By

(Mr.Sarayuth Jittranont)
Assistant General Manager

MULTIPOINT CALIBRATION REPORT

Calibration Date	2-Jul-25	Equipment Name	NOx Analyzer
Manufacturer	HORIBA	Model	APNA-370
Serial No.	7AV89544	Equipment ID	RYG_FS0272
Calibrator Manufacturer	Teledyne API	Model	700
Serial No.	947		
Std. Gas Concentration (PPM)	55.88	Cylinder No.	GN0027222
Cylinder Pressure (psi)	1800	Certified By	Airgas Inc.
Certified Date	9-Feb-22	Expired Date	9-Feb-30

Point	CALIBRATION RESULTS						
	Ideal	Actual NO	Error NO	%Error NO	Actual NOx	Error NOx	%Error NOx
ZERO	0.00	0.05	0.05	0.05	0.10	0.10	0.10
1	100.00	99.10	-0.90	-0.90	100.10	0.10	0.10
2	200.00	198.50	-1.50	-0.75	199.50	-0.50	-0.25
3	300.00	298.60	-1.40	-0.47	300.50	0.50	0.17
4	400.00	398.90	-1.10	-0.28	398.70	-1.30	-0.33
AVERAGE (%)				-0.47			-0.04

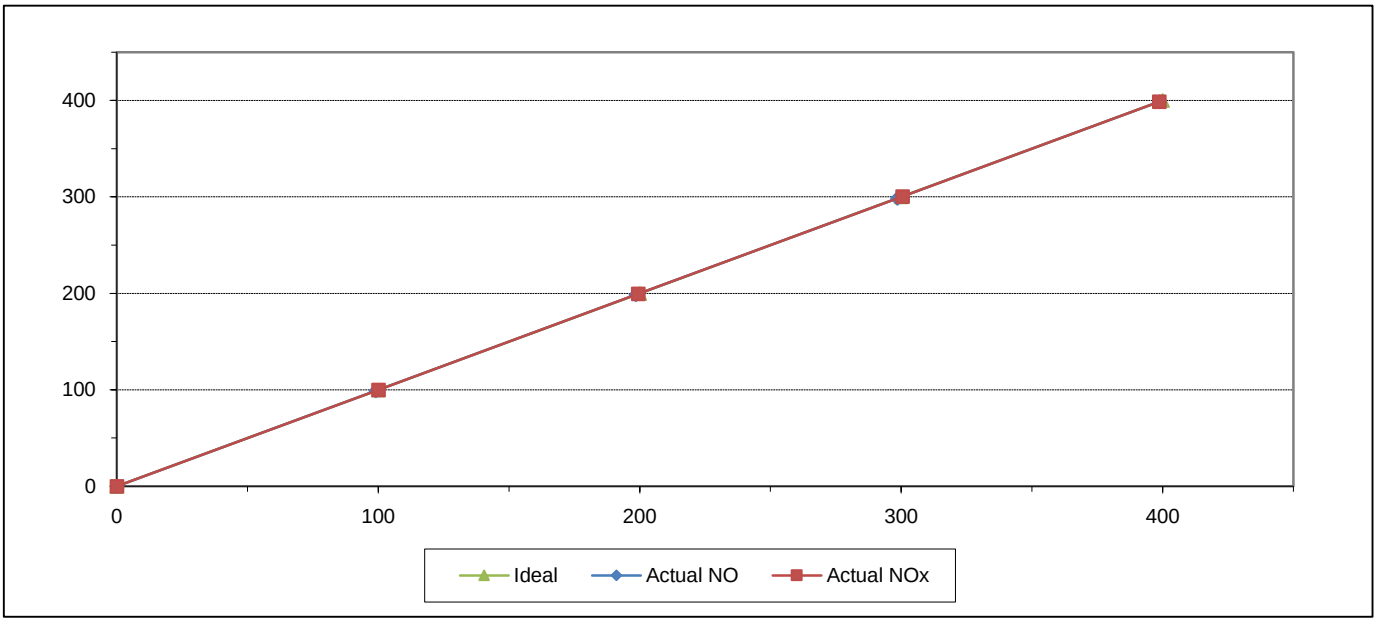

Calibrated By

(Mr.Jirawut Sakarn)
Field Environmental Scientist (3)

Approved By

(Mr.Sarayuth Jittranont)
Assistant General Manager

MULTIPOINT CALIBRATION REPORT

Calibration Date	3-Jul-25	Equipment Name	NOx Analyzer
Manufacturer	HORIBA	Model	APNA-370
Serial No.	T2T8YRLL	Equipment ID	RYG_FS0457
Calibrator Manufacturer	Teledyne API	Model	700
Serial No.	947		
Std. Gas Concentration (PPM)	55.88	Cylinder No.	GN0027222
Cylinder Pressure (psi)	1800	Certified By	Airgas Inc.
Certified Date	9-Feb-22	Expired Date	9-Feb-30

Point	CALIBRATION RESULTS						
	Ideal	Actual NO	Error NO	%Error NO	Actual NOx	Error NOx	%Error NOx
ZERO	0.00	0.10	0.10	0.10	0.10	0.10	0.10
1	100.00	98.30	-1.70	-1.70	100.30	0.30	0.30
2	200.00	198.40	-1.60	-0.80	199.80	-0.20	-0.10
3	300.00	298.70	-1.30	-0.43	298.50	-1.50	-0.50
4	400.00	398.60	-1.40	-0.35	400.50	0.50	0.13
AVERAGE (%)				-0.64			-0.01

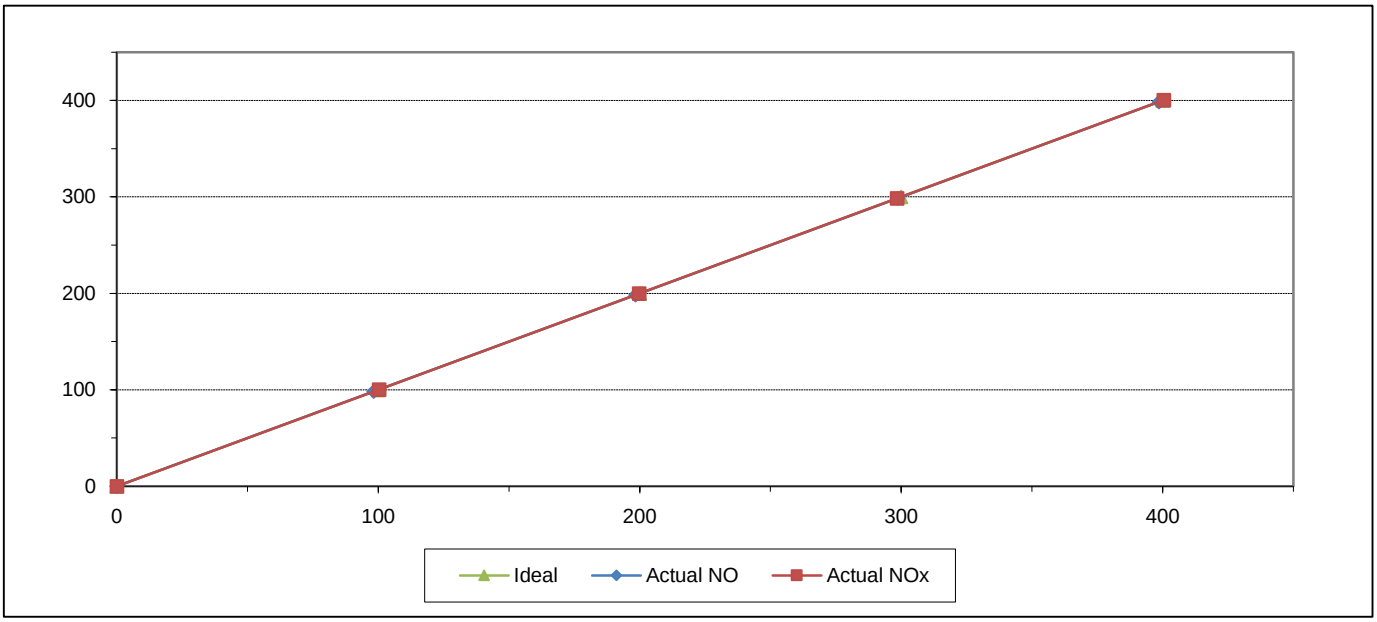

Calibrated By

(Mr.Jirawut Sakarn)
Field Environmental Scientist (3)

Approved By

(Mr.Sarayuth Jittranont)
Assistant General Manager

JIRANATEE ASSOCIATES CO.,LTD.

Jiranatee Associates Co.,Ltd
63/14-15, 67/35-36
Petchkasem 7,7/1, Rd. Watthapra, Bangkokyai,
Bangkok 10600 (Thailand)
Tel: +6608680812
Mobile: +66863999453
E-mail: jnac-calibration@jiranatee.com
Web site: www.jiranatee.com

Accredited calibration laboratory
ISO/IEC 17025:2017
NSC-TISI-TIS 17025
CALIBRATION 0367

Air speed measurement laboratory
Calibration services department.

NSC – TISI – TIS 17025
CALIBRATION 0367

Certificate Number
CWS-057-67

CERTIFICATE OF CALIBRATION

REVIEW BY .....
APPROVED BY .....
NEXT CAL DATE 29 Apr 2026

MEASUREMENT ITEM	: Cup anemometer
MANUFACTURER	: Novalynx
MODEL/TYPE	: Sensor: WS-02F Data logger: 200-WS-25LB
SERIAL NUMBER	: Sensor: WSD-A5375 Data logger: A5375
ID NUMBER	: RYG_FS0413
CONDITION AS-RECEIVED	: Used item
CUSTOMER	: ALS laboratory group (Thailand) Co., Ltd. 104 Phatthanakan 40, Phatthanakan Rd, Khwaeng Suan Luang, Khet Suan Luang, Bangkok 10250 Thailand.
RECEIVED DATE	: 18 Oct 2024
MEASUREMENT DATE	: 29 Oct 2024
ISSUE DATE	: 29 Oct 2024

ENVIRONMENTAL CONDITIONS:
Ambient condition in the laboratory are as follow:

Temperature	: 23.0 ± 3.0	°C
Relative Humidity	: 55.0 ± 15.0	%RH
Atmospheric Pressure	: 1010± 10	hPa

PLACE OF CALIBRATION : Eiffel-type wind tunnel of Jiranatee Associates Co., Ltd.

CALIBRATION CONDITIONS

: Wind tunnel cross-section area[1]	900	cm^2
Wind direction frontal area[2]	100	cm^2
Diameter of mounting pipe[3]	-	mm
Blockage ratio of test object[4]	0.111	[-]

Preconditioning : 24 hours at ambient conditions.
Measurement Condition : The average values during measurement are (22.9) °C, (42.4) %RH and (1004.2) hPa.

Calibration procedure:
The Cup anemometer was calibrated against Standard air velocity transducer model: 8455-12 and pitot tube with precision differential pressure meter model: DPM2500 in an close test-section of Eiffel-type wind tunnel with 900 cm^2 cross test section area. The WI-CL-007 based on IEC 61400-12-1, Wind energy generation systems – Part 12-1: Power performance measurements of electricity producing wind turbines, March 2017 was used as a calibration guideline.

Traceability:
This certificate provides a traceability of The measurement to recognized the national standards, and to realization of the international system of units (SI) through the NIMT (National Metrology Institute of Thailand) via Certificate number: MW-0007-24 and MW-0065-24

Uncertainty of Measurement:
The reported uncertainty of measurement is based on the standard uncertainty multiplied by a coverage factor k=2, Which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty has been determined in accordance with the GUM 'Evaluation of measurement data - Guide to the expression of uncertainty in measurement'

TABULATION OF RESULTS:
The table on next page give the measured values.

Calibrated by:
☑ Mr. Sorawit Thachalad
☐ Miss Jittraporn Lertsomphol

JIRANATEE ASSOCIATES CO.,LTD.

Approved signatory: .....
Mr. Parinya Booncharoen
Calibration Department Manager

Remark:
[1] Nozzle cross-section area of the wind tunnel
[2] Projected cross-section area of the tested object include mounting pipe
[3] Diameter of mounting pipe
[4] Ratio [2] to [1]

THIS CERTIFICATE OF CALIBRATION MAY NOT BE REPRODUCED EXCEPT IN FULL UNLESS PERMISSION FOR REPRODUCTION HAS BEEN OBTAINED IN WRITING FROM THE LABORATORY

Certificate Number
CWS-057-67

MEASUREMENT RESULTS [5]

The Cup anemometer, Unit Under Calibration (UUC) was exercise at 10 m/s for 5 minutes prior to calibration being performed. The standard air velocity 0.5 m/s to 5 m/s was calculated by a standard air velocity transducer which was installed 50 mm away from wind tunnel nozzle and installed 40 mm away from top of the test section and the standard air velocity 5 m/s to 30 m/s was calculated by a pitot tube with precision differential pressure meter which was installed 50 mm away from wind tunnel nozzle and installed 40 mm away from top of the test section, UUC was mounted on a round vertical tube of the lower plate at center of test section. The calibration was carried out under both rising and falling air velocity in the range of 1 m/s to 16 m/s at calibration interval of 1 m/s. The results of calibration and associated measurement uncertainties are reported in the table below.

v_{std} [6] (m/s)	Temp. wind tunnel (°C)	Temp. room (°C)	v_{uuc} [7] (m/s)	Error (m/s)	*U (k=2)* (m/s)
1.004	23.00	22.90	0.9	-0.1	0.31
2.178	22.80	22.90	2.0	-0.2	0.31
3.006	22.90	22.90	2.9	-0.1	0.31
4.200	22.92	22.90	4.0	-0.2	0.31
4.93	22.70	22.90	4.9	0.0	0.31
5.95	22.72	22.90	5.9	-0.1	0.31
7.00	22.78	22.90	7.0	0.0	0.31
7.95	22.64	22.90	7.9	-0.1	0.31
8.94	22.88	22.90	9.0	0.0	0.31
9.94	22.94	22.90	10.1	0.1	0.31
11.07	22.54	22.90	11.1	0.0	0.31
12.00	22.90	22.90	12.0	0.0	0.31
12.93	22.64	22.90	13.0	0.1	0.31
13.92	22.84	22.90	14.1	0.1	0.31
14.95	22.70	22.90	15.1	0.2	0.33
15.94	22.70	22.90	16.3	0.3	0.32

Remark:

[5] Calibration results only count for the tested circumstances and environmental conditions during which calibration took place

[6] Velocity of standard

[7] Velocity of Unit Under Calibration

PHOTO OF CALIBRATION SET-UP

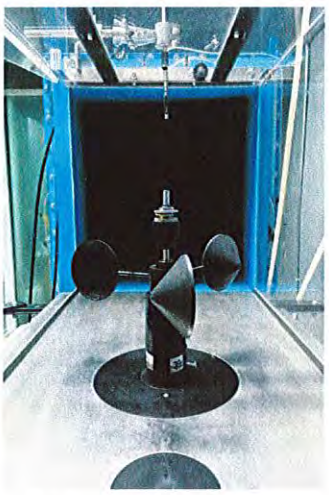

Calibration set-up of the Cup anemometer calibration in the wind tunnel of Jiranatee Associates Co., Ltd. The Cup anemometer shown may differ from the calibrated one. Remark: The proportion of the set- up is not true to scale due to imaging geometry.

End of Certificate of Calibration

JIRANATEE ASSOCIATES CO., LTD.

Jiranatee Associates Co., Ltd.

JIRANATEE ASSOCIATES CO.,LTD.

Jiranatee Associates Co.,Ltd
63/14-15, 67/35-36
Petchkasem 7,7/1, Rd. Watthapra, Bangkokyai,
Bangkok10600(Thailand)
Tel: +6608680812
Mobile: +66863999453
E-mail: jnac-calibration@jiranatee.com
Web site: www.jiranatee.com

Accredited calibration laboratory
ISO/IEC 17025:2017
NSC-TISI-TIS 17025
CALIBRATION 0367

Air speed measurement laboratory
Calibration services department.

NSC – TISI – TIS 17025
CALIBRATION 0367

Certificate Number
CWS-053-67

CERTIFICATE OF CALIBRATION

MEASUREMENT ITEM : Cup anemometer
MANUFACTURER : Novalynx
MODEL/TYPE : Sensor: WS-02F
Data logger: 200-WS-25DL
SERIAL NUMBER : Sensor: WSD-A4987
Data logger: A4987
ID NUMBER : RYG_FS0089
CONDITION AS-RECEIVED : Used item
CUSTOMER : ALS laboratory group (Thailand) Co., Ltd.
104 Phatthanakan 40, Phatthanakan Rd, Khwaeng Suan Luang,
Khet Suan Luang, Bangkok 10250 Thailand.

RECEIVED DATE : 30 Sep 2024
MEASUREMENT DATE : 07 Oct 2024
ISSUE DATE : 07 Oct 2024

ENVIRONMENTAL CONDITIONS:
Ambient condition in the laboratory are as follow:

Temperature	: 23.0 ± 3.0	°C
Relative Humidity	: 55.0 ± 15.0	%RH
Atmospheric Pressure	: 1010± 10	hPa

PLACE OF CALIBRATION : Eiffel-type wind tunnel of Jiranatee Associates Co., Ltd.

CALIBRATION CONDITIONS

: Wind tunnel cross-section area[1]	900	cm^2
Wind direction frontal area[2]	100	cm^2
Diameter of mounting pipe[3]	-	mm
Blockage ratio of test object[4]	0.111	[-]

Preconditioning : 24 hours at ambient conditions.
Measurement Condition : The average values during measurement are (23.0) °C, (42.6) %RH and (1009.0) hPa.

Calibration procedure:
The Cup anemometer was calibrated against Standard air velocity transducer model: 8455-12 and pitot tube with precision differential pressure meter model: DPM2500 in an close test-section of Eiffel-type wind tunnel with 900 cm^2 cross test section area. The WI-CL-007 based on IEC 61400-12-1, Wind energy generation systems – Part 12-1: Power performance measurements of electricity producing wind turbines, March 2017 was used as a calibration guideline.

Traceability:
This certificate provides a traceability of The measurement to recognized the national standards, and to realization of the international system of units (SI) through the NIMT (National Metrology Institute of Thailand) via Certificate number: MW-0007-24 and MW-0055-23

Uncertainty of Measurement:
The reported uncertainty of measurement is based on the standard uncertainty multiplied by a coverage factor k=2, Which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty has been determined in accordance with the GUM 'Evaluation of measurement data - Guide to the expression of uncertainty in measurement'

REVIEW BY Worakorn P.
APPROVED BY
NEXT CAL. DATE 7/4/26

TABULATION OF RESULTS:
The table on next page give the measured values.

Calibrated by:
☑ Mr. Sorawit Thachalad
☐ Miss Jittraporn Lertsomphol

JIRANATEE ASSOCIATES CO.,LTD

Approved signatory: .....
Mr. Parinya Booncharoen
Calibration Department Manager

Remark:
[1] Nozzle cross-section area of the wind tunnel
[2] Projected cross-section area of the tested object include mounting pipe
[3] Diameter of mounting pipe
[4] Ratio [2] to [1]

THIS CERTIFICATE OF CALIBRATION MAY NOT BE REPRODUCED EXCEPT IN FULL UNLESS PERMISSION FOR REPRODUCTION HAS BEEN OBTAINED IN WRITING FROM THE LABORATORY

Certificate Number
CWS-053-67

MEASUREMENT RESULTS [5]

The Cup anemometer, Unit Under Calibration (UUC) was exercise at 10 m/s for 5 minutes prior to calibration being performed. The standard air velocity 0.5 m/s to 5 m/s was calculated by a standard air velocity transducer which was installed 50 mm away from wind tunnel nozzle and installed 40 mm away from top of the test section and the standard air velocity 5 m/s to 30 m/s was calculated by a pitot tube with precision differential pressure meter which was installed 50 mm away from wind tunnel nozzle and installed 40 mm away from top of the test section, UUC was mounted on a round vertical tube of the lower plate at center of test section. The calibration was carried out under both rising and falling air velocity in the range of 1 m/s to 16 m/s at calibration interval of 1 m/s. The results of calibration and associated measurement uncertainties are reported in the table below.

v_{std} [6] (m/s)	Temp. wind tunnel (°C)	Temp. room (°C)	v_{UUC} [7] (m/s)	Error (m/s)	*U (k=2)* (m/s)
1.002	22.94	23.00	0.9	-0.1	0.31
2.223	23.12	23.00	2.0	-0.2	0.31
3.093	22.82	23.00	3.0	-0.1	0.31
4.236	22.84	23.00	4.0	-0.2	0.31
4.95	22.96	23.00	5.0	0.0	0.31
5.96	22.86	23.00	6.0	0.1	0.31
7.03	22.84	23.00	7.0	0.0	0.31
7.96	22.92	23.00	8.0	0.0	0.31
8.97	22.60	23.00	9.2	0.2	0.31
9.96	22.70	23.00	10.1	0.2	0.31
11.09	22.72	23.00	11.3	0.2	0.31
12.02	22.70	23.00	12.2	0.2	0.31
12.94	22.84	23.00	13.3	0.3	0.31
13.92	22.80	23.00	14.3	0.4	0.31
14.99	22.90	23.00	15.3	0.3	0.31
15.96	22.90	23.00	16.2	0.2	0.35

Remark:

[5] Calibration results only count for the tested circumstances and environmental conditions during which calibration took place

[6] Velocity of standard

[7] Velocity of Unit Under Calibration

PHOTO OF CALIBRATION SET-UP

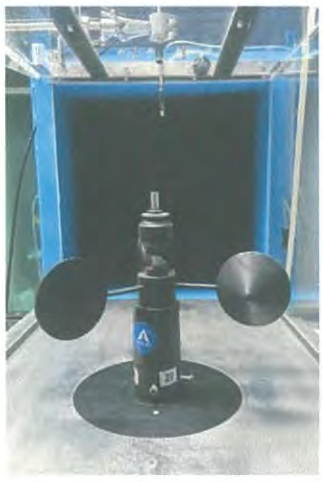

Calibration set-up of the Cup anemometer calibration in the wind tunnel of Jiranatee Associates Co., Ltd. The Cup anemometer shown may differ from the calibrated one. Remark: The proportion of the set- up is not true to scale due to imaging geometry.

End of Certificate of Calibration

JIRANATEE ASSOCIATES CO.,LTD

Jiranatee Associates Co., Ltd.

JIRANATEE ASSOCIATES CO.,LTD.

Jiranatee Associates Co.,Ltd
63/14-15, 67/35-36
Petchkasem 7,7/1, Rd. Watthapra, Bangkokyai,
Bangkok 10600 (Thailand)
Tel: +6608680812
Mobile: +66863999453
E-mail: jnac-calibration@jiranatee.com
Web site: www.jiranatee.com

Accredited calibration laboratory
ISO/IEC 17025:2017
NSC-TISI-TIS 17025
CALIBRATION 0367

Wind direction measurement laboratory
Calibration services department.

NSC – TISI – TIS 17025
CALIBRATION 0367

Certificate Number
CWD-053-67

CERTIFICATE OF CALIBRATION

MEASUREMENT ITEM : Wind Direction Sensor
MANUFACTURER : Novalynx
MODEL/TYPE : Sensor: WS-02F
Data logger: 200-WS-25DL
SERIAL NUMBER : Sensor: WSD-A4987
Data logger: A4987
ID NUMBER : RYG_FS0089
CONDITION AS-RECEIVED : Used item
CUSTOMER : ALS laboratory group (Thailand) Co., Ltd.
104 Phatthanakan 40, Phatthanakan Rd, Khwaeng Suan Luang,
Khet Suan Luang, Bangkok 10250 Thailand.

RECEIVED DATE : 30 Sep 2024
MEASUREMENT DATE : 07 Oct 2024
ISSUE DATE : 07 Oct 2024

ENVIRONMENTAL CONDITIONS:
Ambient condition in the laboratory are as follow:

Temperature	: 23.0 ± 3.0	°C
Relative Humidity	: 55.0 ± 15.0	%RH
Atmospheric Pressure	: 1010± 10	hPa

PLACE OF CALIBRATION : Eiffel-type wind tunnel of Jiranatee Associates Co., Ltd.

CALIBRATION CONDITION

: Wind tunnel cross-section area[1]	900	cm^2
Wind direction frontal area[2]	129	cm^2
Diameter of mounting pipe[3]	-	mm
Blockage ratio of test object[4]	0.143	[-]

Preconditioning : 24 hours at ambient conditions.
Measurement Condition : The average values during measurement are (23.3)°C, (46.1) %RH and (1007.5) hPa.

Calibration procedure:
The wind direction sensor was calibrated against Standard Rotary Encoder model: AX4009TS-DM04-P3-S-U0 in an close test-section of Eiffel-type wind tunnel with 900 cm^2 cross test section area. The WI-CL-008 based on IEC 61400-12-1, Wind energy generation systems – Part 12-1: Power performance measurements of electricity producing wind turbines, March 2017 was used as a calibration guideline.

Traceability:
This certificate provides a traceability of The measurement to recognized the national standards, and to realization of the international system of units (SI) through the NIMT (National Metrology Institute of Thailand) via Certificate number: DA-0036-23.

Uncertainty of Measurement:
The reported uncertainty of measurement is based on the standard uncertainty multiplied by a coverage factor k=2, Which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty has been determined in accordance with the GUM 'Evaluation of measurement data - Guide to the expression of uncertainty in measurement'

TABULATION OF RESULTS:
The table on next page give the measured values.

Calibrated by:
☑ Mr. Sorawit Thachalad
☐ Miss Jittraporn Lertsomphol

JNAC JIRANATEE ASSOCIATES CO.,LTD

Approved signatory: .....
Mr. Parinya Booncharoen
Calibration Department Manager

Remark:
[1] Nozzle cross-section area of the wind tunnel
[2] Projected cross-section area of the tested object include mounting pipe
[3] Diameter of mounting pipe
[4] Ratio [2] to [1]

THIS CERTIFICATE OF CALIBRATION MAY NOT BE REPRODUCED EXCEPT IN FULL UNLESS PERMISSION FOR REPRODUCTION HAS BEEN OBTAINED IN WRITING FROM THE LABORATORY

Certificate Number
CWD-053-67

MEASUREMENT RESULTS [5]

The wind direction sensor was calibrated against standard rotary encoder by comparison method. During calibration, the measurement was carried out at 45° intervals in clockwise and counterclockwise directions after offset adjustment has been made. The flow speed of wind tunnel (usually 5 m/s) is kept constant while the sensor is rotated around its vertical axis. The results of calibration and associated measurement uncertainties are reported in the table below.

Air speed	D_{std} [6]	D_{uuc} [7]	Error	U (k=2)
m/s	Degree (°)	Degree (°)	Degree (°)	Degree (°)
5.04	0.000	0	0	0.80
	45.000	42	-3	0.80
	90.000	88	-2	0.80
	135.000	134	-1	0.80
	180.000	180	0	0.80
	225.000	228	3	0.80
	270.000	274	4	0.80
	315.000	317	2	0.80

Remark:

[5] Calibration results only count for the tested circumstances and environmental conditions during which calibration took place

[6] Direction of standard

[7] Direction of Unit Under Calibration

End of Certificate of Calibration

Jiranatee Associates Co., Ltd.

JIRANATEE ASSOCIATES CO.,LTD.

Jiranatee Associates Co.,Ltd
63/14-15, 67/35-36
Petchkasem 7,7/1, Rd. Watthapra, Bangkokyai,
Bangkok 10600 (Thailand)
Tel: +6608680812
Mobile: +66863999453
E-mail: jnac-calibration@jiranatee.com
Web site: www.jiranatee.com

Accredited calibration laboratory
ISO/IEC 17025:2017
NSC-TISI-TIS 17025
CALIBRATION 0367

Air speed measurement laboratory
Calibration services department.

NSC – TISI – TIS 17025
CALIBRATION 0367

Certificate Number
CWS-058-67

CERTIFICATE OF CALIBRATION

REVIEW BY .....

APPROVED BY.....

NEXT CAL DATE..... 29 Apr 2026

MEASUREMENT ITEM : Cup anemometer
MANUFACTURER : Novalynx
MODEL/TYPE : Sensor: WS-02F
Data logger: 200-WS-25LB
SERIAL NUMBER : Sensor: WSD-A5376
Data logger: A5376
ID NUMBER : RYG_FS0414
CONDITION AS-RECEIVED : Used item
CUSTOMER : ALS laboratory group (Thailand) Co., Ltd.
104 Phatthanakan 40, Phatthanakan Rd, Khwaeng Suan Luang,
Khet Suan Luang, Bangkok 10250 Thailand.

RECEIVED DATE : 18 Oct 2024
MEASUREMENT DATE : 29 Oct 2024
ISSUE DATE : 29 Oct 2024

ENVIRONMENTAL CONDITIONS:
Ambient condition in the laboratory are as follow:

Temperature	: 23.0 ± 3.0	°C
Relative Humidity	: 55.0 ± 15.0	%RH
Atmospheric Pressure	: 1010± 10	hPa

PLACE OF CALIBRATION : Eiffel-type wind tunnel of Jiranatee Associates Co., Ltd.

CALIBRATION CONDITIONS

: Wind tunnel cross-section area[1]	900	cm^2
Wind direction frontal area[2]	100	cm^2
Diameter of mounting pipe[3]	-	mm
Blockage ratio of test object[4]	0.111	[-]

Preconditioning : 24 hours at ambient conditions.
Measurement Condition : The average values during measurement are (23.0) °C, (46.8) %RH and (1003.6) hPa.

Calibration procedure:
The Cup anemometer was calibrated against Standard air velocity transducer model: 8455-12 and pitot tube with precision differential pressure meter model: DPM2500 in an close test-section of Eiffel-type wind tunnel with 900 cm^2 cross test section area. The WI-CL-007 based on IEC 61400-12-1, Wind energy generation systems – Part 12-1: Power performance measurements of electricity producing wind turbines, March 2017 was used as a calibration guideline.

Traceability:
This certificate provides a traceability of The measurement to recognized the national standards, and to realization of the international system of units (SI) through the NIMT (National Metrology Institute of Thailand) via Certificate number: MW-0007-24 and MW-0065-24

Uncertainty of Measurement:
The reported uncertainty of measurement is based on the standard uncertainty multiplied by a coverage factor k=2, Which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty has been determined in accordance with the GUM 'Evaluation of measurement data - Guide to the expression of uncertainty in measurement'

TABULATION OF RESULTS:
The table on next page give the measured values.

Calibrated by:
☑ Mr. Sorawit Thachalad
☐ Miss Jittraporn Lertsomphol

JIRANATEE ASSOCIATES CO.,LTD.

Approved signatory: .....
Mr. Parinya Booncharoen
Calibration Department Manager

Remark:
[1] Nozzle cross-section area of the wind tunnel
[2] Projected cross-section area of the tested object include mounting pipe
[3] Diameter of mounting pipe
[4] Ratio [2] to [1]

THIS CERTIFICATE OF CALIBRATION MAY NOT BE REPRODUCED EXCEPT IN FULL UNLESS PERMISSION FOR REPRODUCTION HAS BEEN OBTAINED IN WRITING FROM THE LABORATORY

Certificate Number
CWS-058-67

MEASUREMENT RESULTS [5]

The Cup anemometer, Unit Under Calibration (UUC) was exercise at 10 m/s for 5 minutes prior to calibration being performed. The standard air velocity 0.5 m/s to 5 m/s was calculated by a standard air velocity transducer which was installed 50 mm away from wind tunnel nozzle and installed 40 mm away from top of the test section and the standard air velocity 5 m/s to 30 m/s was calculated by a pitot tube with precision differential pressure meter which was installed 50 mm away from wind tunnel nozzle and installed 40 mm away from top of the test section, UUC was mounted on a round vertical tube of the lower plate at center of test section. The calibration was carried out under both rising and falling air velocity in the range of 1 m/s to 16 m/s at calibration interval of 1 m/s. The results of calibration and associated measurement uncertainties are reported in the table below.

v_{std} [6] (m/s)	Temp. wind tunnel (°C)	Temp. room (°C)	v_{UUC} [7] (m/s)	Error (m/s)	*U (k=2)* (m/s)
1.012	22.94	22.95	0.8	-0.2	0.31
2.209	23.00	22.95	2.0	-0.2	0.31
3.050	22.78	22.95	2.9	-0.1	0.31
4.206	22.82	22.95	4.1	-0.1	0.31
4.93	22.90	22.95	5.1	0.2	0.31
5.92	22.90	22.95	6.0	0.1	0.31
7.04	22.60	22.95	7.0	-0.1	0.31
7.96	22.74	22.95	8.0	0.1	0.46
8.96	22.76	22.95	8.9	0.0	0.31
9.96	22.50	22.95	10.0	0.1	0.31
11.08	22.90	22.95	11.1	0.0	0.31
12.01	22.52	22.95	12.0	0.0	0.31
12.96	22.58	22.95	13.1	0.1	0.35
13.94	22.54	22.95	14.0	0.1	0.35
14.98	22.60	22.95	15.0	0.0	0.31
15.98	22.60	22.95	16.1	0.1	0.31

Remark:

[5] Calibration results only count for the tested circumstances and environmental conditions during which calibration took place

[6] Velocity of standard

[7] Velocity of Unit Under Calibration

PHOTO OF CALIBRATION SET-UP

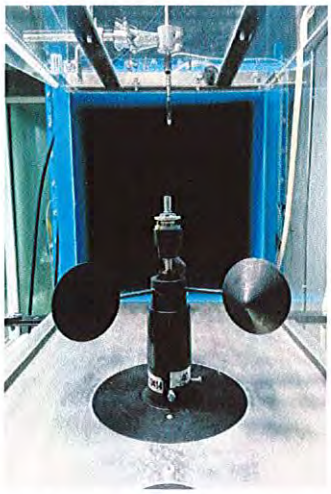

Calibration set-up of the Cup anemometer calibration in the wind tunnel of Jiranatee Associates Co., Ltd. The Cup anemometer shown may differ from the calibrated one. Remark: The proportion of the set- up is not true to scale due to imaging geometry.

End of Certificate of Calibration

NAC
JIRANATEE ASSOCIATES CO., LTD

Jiranatee Associates Co., Ltd.

CONSOLE CONTROL UNIT CALIBRATION TEST REPORT

Calibration of Date : 10-Jul-25
Next Cal. Date : 10-Jan-26

Barometric Pressure (mmHg) : 751.3
Relative Humidity (%) : 43.7
Temperature (C°) : 27.1

Console Control Meter Data

Calibration No. : C-100725-BKK_FS0468
Dry Gas Meter ID : BKK_FS0468
Serial No. : 1302005
Model No. : XC-572-V

Reference Dry Gas Meter Data

Reference Dry Gas Meter ID : BKK_FS1122
Serial No. : A2003240
Correction Factor (Y) : 1.0000
Next Calibration Date : 25 Feb 26

ΔH ($mm.H_2O$)	Θ Minutes	Reference Dry Gas Meter Calibration				Console Control ; Drygas Meter						Dry Gas Meter Correction Factor (Y)	Orifice Calibration Factor ΔH@
		Vr (Liters)			Tr (°C)	Vm (Liters)			Ti (°C)	To (°C)	Avg.Tm (°C)		
		Final	Initial	Total		Final	Initial	Total					
15	12.21	150.00	0.00	150.00	27.0	792201.0	792056.0	145.00	27.0	27.0	27.0	1.0330	45.6797
25	9.23	150.00	0.00	150.00	27.0	792353.0	792207.0	146.00	27.0	27.0	27.0	1.0249	43.5055
50	6.50	150.00	0.00	150.00	28.0	792497.0	792357.0	140.00	28.0	28.0	28.0	1.0662	43.2955
80	5.09	150.00	0.00	150.00	28.0	792658.0	792511.0	147.00	28.0	28.0	28.0	1.0125	42.4787
120	4.11	150.00	0.00	150.00	28.0	792817.0	792670.0	147.00	29.0	29.0	29.0	1.0119	41.4067
											Avg.	1.0297	43.2732

Y : Ratio of reading of reference to dry gas meter : tolerance for individual values ± 0.02 from average .

ΔH@ : Orifice pressure differential that equates to 21.24 lm of air @ 25 C and 760 mm of mercury , mmH2O ; tolerance for individual values ± 5.08 from average .

Procedure; 40 CFR 60,APP A,METH ,SEC 5.3 & 7

Calibrated by: _____
(Mr. Warawut Pubpa)
RYG Field Service Scientist(3)

Approved by: Natthapon Jiengwareewong
(Mr.Natthapol Jiengwareewong)
RYG Field Service Specialist(

DIGITAL TEMPERATURE CALIBRATION DATA SHEET

Calibration Date :	10 Jul 25	Ambient Temperature (°C)	43.7
Calibration sheet No. :	C-100725-BKK_FS0469	Relative Humidity (%) :	27

Digital Temperature ID :	BKK_FS0469	Reference Temperature ID	BKK_FS1144
Serial No. :	1302005	Serial No. :	201090006013
Model :	XC-572-V	Model :	Digicon-CC-VT-MS
		Next Calibrate :	5 Jan 26

Location	Reference Temperature °C	Digital Temperature °C	Error °C	MPE	Pass / Fail
Stack	0	3	3	±3	Pass
	25	27	2	±3	Pass
	50	51	1	±3	Pass
	100	100	0	±3	Pass
	150	148	-2	±3	Pass
	200	198	-2	±3	Pass
	250	247	-3	±3	Pass
	300	298	-2	±3	Pass
	500	497	-3	±3	Pass
Probe	100	100	0	±3	Pass
	120	120	0	±3	Pass
	140	139	-1	±3	Pass
Oven	100	100	0	±3	Pass
	120	120	0	±3	Pass
	140	139	-1	±3	Pass
Filter	100	100	0	±3	Pass
	120	120	0	±3	Pass
	140	139	-1	±3	Pass
Exit	0	1	1	±3	Pass
	10	11	1	±3	Pass
	20	21	1	±3	Pass
Meter	0	0	0	±3	Pass
	25	26	1	±3	Pass
	50	51	1	±3	Pass
AUX	0	0	0	±3	Pass
	25	26	1	±3	Pass
	50	50	0	±3	Pass

MPE : (Maximum permissible error of measurement) ค่าความผิดพลาดสูงสุดของการวัดที่ยอมได้

Calibrated by :

(Mr. Warawut Pubpa)

RYG Field Service Scientist (3)

Approved by : Natthapon Jiengwareewong

(Mr.Natthapol Jiengwareewong)

RYG Field Service Specialist (1)

PROBE NOZZLE DIAMETER

CALIBRATION DATA SHEET

Calibration Date :	10 Jul 25	Nozzle Set ID. :	BKK_FS0474
Calibration Sheet No. : C-100725-BKK_FS0474		Vernier Caliper ID.:	RYG_FS0539

Nozzle ID #	Nozzle Diameter (cm.)			Hi - Lo	$(D_1 + D_2 + D_3) / 3$
	D_1	D_2	D_3	ΔD	D_{avg}
1	0.305	0.300	0.302	0.005	0.302
2	0.451	0.455	0.453	0.004	0.453
3	0.540	0.545	0.535	0.010	0.540
4	0.601	0.602	0.601	0.001	0.601
5	0.758	0.765	0.766	0.008	0.763
6	0.935	0.934	0.935	0.001	0.935
7	1.095	1.092	1.092	0.003	1.093
8	1.260	1.259	1.260	0.001	1.260
9	1.605	1.601	1.610	0.009	1.605

Where :

D_1, D_2, D_3 = There different nozzle diameters at 60 degrees to each other, each measured the nearest 0.025 mm.

ΔD = Maximum distance between any two diameters, must be $\leq$ 0.100 mm.

D_{avg} = $(D_1 + D_2 + D_3) / 3$

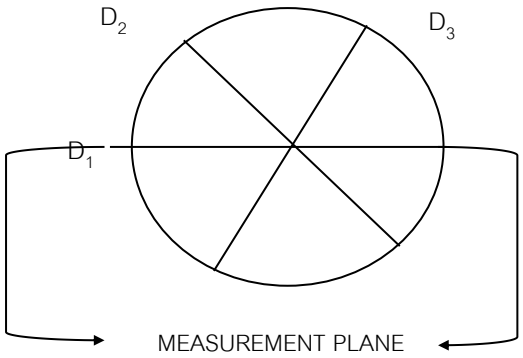

Calibrated by : _____

(Mr. Warawut Pubpa)

RYG Field Services Scientist (3)

Approved by : Natthapon Jiengwareewong

(Mr.Natthapol Jiengwareewong)

RYG Field Services Specialist (1)

Type S Pitot Tube Calibration

Date Calibration	10-Jul-25	**Due Date**	10-Jan-26
Pitot ID	BKK_FS0472	**Inclinometer ID**	BKK_FS1131
Pitot SN		**Vernier ID**	RYG_FS0539

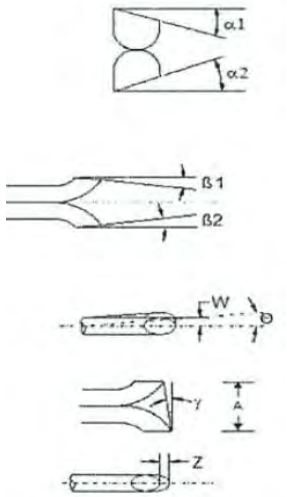

Parameter	Value	Allowable Range	Check
α1	0.9	-10° < α1 < +10°	OK
α2	3.2	-10° < α2 < +10°	OK
β1	-2.3	-5° < β1 < +5°	OK
β2	-0.3	-5° < β2 < +5°	OK
γ	1	-	-
θ	1.9	-	-
Z = A tan γ	0.016	Z ≤ 0.125"	OK
W = A tan θ	0.030	W ≤ 0.031"	OK
Dt	0.310	0.188" to 0.375"	OK
A/2Dt	1.452	1.05 ≤ PA/Dt ≤ 1.5	OK
A	0.9	2.1Dt ≤ A ≤ 3Dt	OK

Certify that pitot tube/porbe meets or exceeds all specifications, crieria and/or applicable design features and is hereby assigned a pitot tube certification fact of 0.84 . See 40 CFR Pt. 60, App. A,EPA Method 2.

Calibrated by : _____

(Mr. Warawut Pubpa)

RYG Field Services Scientist (3)

Approved By : Natthapon Jiengwareewong

(Mr.Natthapol Jiengwareewong)

RYG Field Services Specialist (1)

ENTECH
Where Solutions Begin

Calibration Certificate

NSC-TISI-TIS 17025
CALIBRATION 0157

Certificate No: G 680210
Date of issue : 25-Mar-25

Instrument description	:	Flue Gas Analyzer
Instrument model	:	Testo 350 New
Instrument serial no.	:	62087344/1119
Control unit serial no.	:	03401649/1119
ID no. or control no.	:	RYG_FS0464
Manufacturer	:	Testo SE & Co. KGaA
Probe description	:	-
Probe model	:	-
Probe serial no.	:	-
Customer name	:	ALS LABORATORY GROUP (THAILAND) CO.,LTD.
Customer address	:	104 Phatthanakan 40, Phatthanakan Road, Khwaeng Phatthanakan, Khet Suan Luang, Bangkok, 10250 Thailand
Total pages of certificate	:	3 Pages
Receiving no.	:	L-250946
Receiving date.	:	18-Mar-25
Parameter of calibration	:	Gas Calibration(Oxygen 2.50,9.984,21.02 %vol, Carbon Monoxide 80.45,302,1007 ppm, Nitrogen Dioxide 30.68,81.8,202.6 ppm, Nitric Oxide 30.0,151.8,322.5 ppm, Sulphur Dioxide 50.36,100.7,600.8 ppm)
Condition of UUC.	:	Used
Ambient condition	:	All of the Measurment ware caried out the stabilized labotary Temperature : 23 ±5 °C Humidity : 55 ± 15 %RH
Calibration place	:	17/121 Soi Ngamwongwan 47 Yaek 48, Toongsonghong, Laksi, Bangkok 10210 THAILAND
Calibration procedure no	:	This instrument was calibrated by comparison with Standard gas mixture according to calibration Work Instruction no. WI-CL-28-C

REVIEW BY .....

APPROVED BY.....

NEXT CAL DATE....23/ 03/ 2026.....

The calibration certificate expanded uncertainty of measurement is stated as the standard uncertainty of measurent Multiplied by coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

This certificate is applied only to item under test Environmental condition.

This Calibration Certificate may not be reporduced other than in full except with the permission of the issuing laboratory. Calibration certificates without signature and seal not valid and The results relate only to the items tested/calibrated.

This calibration certificate documents are tracebility to national standards, which realize measurement according to the International System of Units (SI).

Date of calibration : 24-Mar-25

Mr. Kwanchai Khamdoung
Calibration Technician

Mrs. Nongluck Wongsettee
Technical Manager

Entech Industrial Solution Co.,Ltd.
17/121 Soi Ngamwongwan 47 Yaek 48, Toongsonghong, Laksi, Bangkok 10210 THAILAND Tel. 0-2779-8888 Calibration@entech.co.th
Tax ID : 0105536035591 www.entech.co.th

Certificate No.: G 680210

Standard References (Table 1)

Standard	Certificate No.	Vendor	Due date
Oxygen (O2) 2.50 % Vol	2412/23	Linde	27-Aug-27
Oxygen (O2) 9.984 % Vol	CG-0113-24	Nimt	01-Aug-29
Oxygen (O2) 21.02 % Vol	CG-0041-22	Nimt	10-Feb-27
Carbon monoxide (CO) 80.45 ppm	CG-0132-24	Nimt	10-Sep-29
Carbon monoxide (CO) 302 ppm	1915/23	Linde	16-Jun-25
Carbon monoxide (CO) 1007 ppm	1870/24	Linde	17-Jun-26
Nitrogen Dioxide (NO2) 30.68 ppm	2832/24	Linde	08-Sep-26
Nitrogen Dioxide (NO2) 81.8 ppm	2330/24	Linde	01-Aug-26
Nitrogen Dioxide (NO2) 202.6 ppm	3794/24	Linde	23-Dec-26
Nitric Oxide (NO) 30.0 ppm	CG-0065-24	Nimt	06-May-26
Nitric Oxide (NO) 151.8 ppm	0404/25	Linde	09-Feb-27
Nitric Oxide (NO) 322.5 ppm	1974/23	Linde	17-Jul-25
Sulphur Dioxide (SO2) 50.36 ppm	2004/23	Linde	17-Jul-25
Sulphur Dioxide (SO2) 100.7 ppm	2662/24	Linde	25-Aug-26
Sulphur Dioxide (SO2) 600.8 ppm	2003/23	Linde	17-Jul-25

Measured room conditions

Temperature : 22.7 °C Humidity : 62.6 %RH Pressure : 1010.5 mbar

Calibration conditions

Gas Temperature : 23 °C Flow rate : 1,300 ml/min Gas pressure : 1016.2 mbar

Calibration Results (Befor adjustment) (Table 2)

Parameter of Standard	Standard Values	Mean of UUC	Error	Uncertainty (±)
O2 (%Vol)	2.50	2.46	-0.04	0.15
O2 (%Vol)	9.984	9.95	-0.034	0.20
O2 (%Vol)	21.02	21.08	0.06	0.30
CO (ppm)	80.45	81	0.55	3.0
CO (ppm)	302	302	0	6.0
CO (ppm)	1007	1010	3	12
NO2 (ppm)	30.68	26.9	-3.78	8.0
NO2 (ppm)	81.8	67.1	-14.7	8.0
NO2 (ppm)	202.6	181.3	-21.3	12
NO (ppm)	30.0	24	-6.0	8.0
NO (ppm)	151.8	145	-6.8	8.0
NO (ppm)	322.5	302	-20.5	12
SO2 (ppm)	50.36	48	-2.36	6.0
SO2 (ppm)	100.7	97	-3.7	6.0
SO2 (ppm)	600.8	589	-11.8	13

Entech Industrial Solution Co.,Ltd.
17/121 Soi Ngamwongwan 47 Yaek 48, Toongsonghong, Laksi, Bangkok 10210 THAILAND Tel. 0-2779-8888 Calibration@entech.co.th
Tax ID : 0105536035591 www.entech.co.th

Calibration Results (After adjustment) (Table 3)

Parameter of Standard	Standard Values	Mean of UUC	Error	Uncertainty (±)
O2 (%Vol)	2.50	2.46	-0.04	0.15
O2 (%Vol)	9.984	9.95	-0.034	0.20
O2 (%Vol)	21.02	21.08	0.06	0.30
CO (ppm)	80.45	81	0.55	3.0
CO (ppm)	302	302	0	6.0
CO (ppm)	1007	1010	3	12
NO2 (ppm)	30.68	29.4	-1.28	8.0
NO2 (ppm)	81.8	79.7	-2.1	8.0
NO2 (ppm)	202.6	199.2	-3.4	12
NO (ppm)	30.0	30	0.0	8.0
NO (ppm)	151.8	153	1.2	8.0
NO (ppm)	322.5	324	1.5	12
SO2 (ppm)	50.36	50	-0.36	6.0
SO2 (ppm)	100.7	101	0.3	6.0
SO2 (ppm)	600.8	599	-1.8	13

Remark : 1 cmol/mol = 1 %vol. 1 µmol/mol = 1 ppm., Sensor CO New.

End of Report

Entech Industrial Solution Co.,Ltd.
17/121 Soi Ngamwongwan 47 Yaek 48, Toongsonghong, Laksi, Bangkok 10210 THAILAND Tel. 0-2779-8888 Calibration@entech.co.th
Tax ID : 0105536035591 www.entech.co.th

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7/139 MOO 13, SOI SUNTINAKORN 11 TAMBON BANG KAEO,
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL: (66)0-2116-5860-1 FAX: (66)0-2116-7140

Certificate of Calibration

Customer

Certificate No : 25-AFM-023

Name : ALS Laboratory Group Thailand Co., Ltd.

Request No : Req-2025-0169

Address : 104 Soi Phatthanakan 40, Phatthanakan Road, Suan Luang, Bangkok 10250

Unit Under Calibration Details

Measurement Item : Air Flow Meter

Manufacturer : Mesa Labs

Accuracy : 1% of Reading

Model : 200-510L

Sensor Model : -

Serial Number : 130027

Sensor Serial Number : -

ID : RYG_FS0208

Instrument Status : Used

Location of Calibration : LAB 4 AIR VELOCITY METER

REVIEW BY .....

APPROVED BY .....

NEXT CAL DATE.....26/ 01/ 26.....

Calibration Environment and Details

Temperature : 23 ˚C ± 3 ˚C

Humidity : 55 %RH ± 20 %RH

Barometric Pressure : 1013 hPa ± 10 hPa

Received Date : 21 January 2025

Calibration Date : 27 January 2025

Calibration Procedure : In-house method CP-AFM-01 by Comparison technique with Standard Primary Flow Calibrator

Reference Standard	Model	Serial Number	Traceble	Due Calibration
Air Flow Meter	Gilibrator 3 Low flow	18501010006	Sensidyne	6 August 2025
Air Flow Meter	Gilibrator 3 Standard flow	19031011003	Sensidyne	2 August 2025
Temperature meter	GT 11	08000057	Qreborn	1 March 2025
Pressure meter	CPG2400	41000KDU/651882	TPA	21 October 2025

Traceability :

This Certificate is traceable to SI Unit through Sensidyne A2LA Accreditation No. 3943.01

Note :

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor k = 2, providing a level of confidence approximately 95 %.

Calibration By :

Mr. Noppadon Luangart

Service Calibration Engineer

Approved By :

Mr. Pacit Mathavorn

Calibration Engineer Supervisor

Issue Date : 27 January 2025

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7/139 MOO 13, SOI SUNTINAKORN 11 TAMBON BANG KAEO,
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL: (66)0-2116-5860-1 FAX: (66)0-2116-7140

Certificate No : 25-AFM-023

Request No : Req-2025-0169

Result of Calibration : Without Adjustment

Temperature (°C)	Pressure (kPa)	STD (cc/min)	UUC (cc/min)	Error (cc/min)	Uncertainty (cc/min)	MPE (cc/min)	Result
22.50	100.90	20	19.854	-0.1	1.3	0.2	Pass1
22.50	100.90	50	49.732	-0.3	3.3	0.5	Pass1
22.60	100.90	101	100.77	-0.2	2.8	1.0	Pass1
22.70	100.90	151	150.23	-0.8	4.2	1.5	Pass1
22.70	100.90	201	200.39	-0.6	5.6	2.0	Pass1
22.70	100.90	301	300.69	-0.3	8.4	3.0	Pass1
22.80	100.90	400	402.96	3.0	11	4.0	Pass1
23.10	100.90	500	504.62	4.6	7.2	5.0	Pass1

Note STD : Standard UUC : Unit Under Calibration

- UUC Reference Condition : At atmospheric pressure and room temperature condition
- Flow Rate was corrected for non-standard operating condition by using equation :

$$Q_{meas} = Q_{ref} \times \frac{P_{ref}}{P_{ref}} \times \frac{T_{meas}}{T_{ref}}$$

where Q = Flow Rate P = Absolute Pressure T = Absolute Temperature
Meas = Measurement Condition ref = Standard Condition

* Indicates non accredited

MPE = Maximum Permissible Error (Specified in Manufacturer's Specifications)

N/A = Not Aavailable, Customer does not require a statement of conformity.

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7/139 MOO 13, SOI SUNTINAKORN 11 TAMBON BANG KAEO,
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL: (66)0-2116-5860-1 FAX: (66)0-2116-7140

Certificate No : 25-AFM-023

Request No : Req-2025-0169

Decision Rule for Statements of Conformity

The standard decision rule employed for the statements of conformity to each calibration result will be applied using ILAC-G8:09/2019; Guidelines on the Reporting of Compliance with Specification as following Fig. and statements

Pass = The measurement result plus the expanded uncertainty with a 95% coverage probability were within the limit.

Pass[1] = The measurement result was within the limit. However, a portion of the expanded uncertainty of measurement at 95% exceeds the limit.

Fail[1] = The measurement result was out of the limit. However, a portion of the expanded uncertainty of measurement at 95% is within the limit.

Fail = The measurement result plus the expanded uncertainty with a 95% coverage probability were outside the limit.

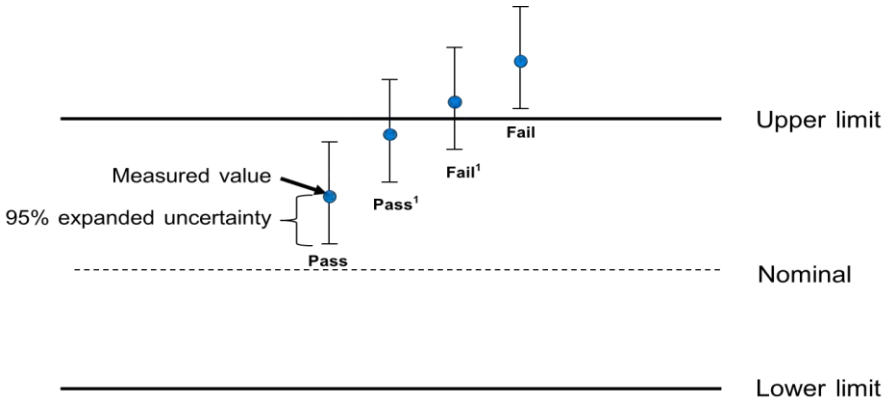

End of Certificate

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7/139 MOO 13, SOI SUNTINAKORN 11 TAMBON BANG KAEO,
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL: (66)0-2116-5860-1 FAX: (66)0-2116-7140

Certificate of Calibration

Customer

Certificate No : 24-AFM-179

Name : ALS Laboratory Group Thailand Co., Ltd.

Request No : Req-2024-1987

Address : 104 Soi Phatthanakan 40, Phatthanakan Road, Suan Luang, Bangkok 10250

Unit Under Calibration Details

Measurement Item : Air Flow Meter

Manufacturer : MesaLabs

Accuracy : 1% of Reading

Model : Defender 510-M

Sensor Model : -

Serial Number : 151114

Sensor Serial Number : -

ID : BKK_FS0614

Instrument Status : Used

Location of Calibration : LAB 4 AIR VELOCITY METER

Calibration Environment and Details

REVIEW BY Narakorn P.
APPROVED BY
NEXT CAL. DATE 9/9/25

Temperature : 23 °C ± 3 °C

Humidity : 55 %RH ± 20 %RH

Barometric Pressure : 1013 hPa ± 10 hPa

Received Date : 30 August 2024

Calibration Date : 9 September 2024

Calibration Procedure : In-house method CP-AFM-01 by Comparison technique with Standard Primary Flow Calibrator

Reference Standard	Model	Serial Number	Traceble	Due Calibration
Air Flow Meter	Gilibrator 3 Low flow	18501010006	Sensidyne	6 August 2025
Air Flow Meter	Gilibrator 3 Standard flow	19031011003	Sensidyne	2 August 2025
Temperature meter	GT 11	08000057	Qreborn	1 March 2025
Pressure meter	CPG2400	41000KDU/651882	TPA	9 November 2024

Traceability :

This Certificate is traceable to SI Unit through Sensidyne A2LA Accreditation No. 3943.01

Note :

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor $k = 2$, providing a level of confidence approximately 95 %.

Calibration By :

Mr. Noppadon Luangart

Service Calibration Engineer

Approved By :

Mr. Pacit Mathavorn

Calibration Engineer Supervisor

Issue Date : 9 September 2024

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7/139 MOO 13, SOI SUNTINAKORN 11 TAMBON BANG KAEO,
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL: (66)0-2116-5860-1 FAX: (66)0-2116-7140

Certificate No : 24-AFM-179

Request No : Req-2024-1987

Result of Calibration : Without Adjustment

Temperature (°C)	Pressure (kPa)	STD (cc/min)	UUC (cc/min)	Error (cc/min)	Uncertainty (cc/min)	MPE (cc/min)	Result
24.70	100.95	100	100.41	0.4	2.8	1.0	N/A
24.90	100.90	502	500.47	-1.5	7.1	5.0	N/A
24.90	100.97	1003	1001.3	-2	14	10.0	N/A
25.00	100.92	2014	2009.9	-4	29	20.1	N/A
25.20	101.03	3043	3058.3	15	44	30.4	N/A
25.30	101.10	4043	4005.1	-38	57	40.4	N/A
25.50	101.15	5052	5003.9	-48	74	50.5	N/A

Note STD : Standard UUC : Unit Under Calibration

- UUC Reference Condition : At atmospheric pressure and room temperature condition
- Flow Rate was corrected for non-standard operating condition by using equation :

$$Q_{meas} = Q_{ref} \times \frac{P_{ref}}{P_{ref}} \times \frac{T_{meas}}{T_{ref}}$$

where Q = Flow Rate P = Absolute Pressure T = Absolute Temperature

Meas = Measurement Condition ref = Standard Condition

* Indicates non accredited

MPE = Maximum Permissible Error (Specified in Manufacturer's Specifications)

N/A = Not Aavailable, Customer does not require a statement of conformity.

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7/139 MOO 13, SOI SUNTINAKORN 11 TAMBON BANG KAEO,
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL: (66)0-2116-5860-1 FAX: (66)0-2116-7140

Certificate No : 24-AFM-179

Request No : Req-2024-1987

Decision Rule for Statements of Conformity

The standard decision rule employed for the statements of conformity to each calibration result will be applied using ILAC-G8:09/2019; Guidelines on the Reporting of Compliance with Specification as following Fig. and statements

Pass = The measurement result plus the expanded uncertainty with a 95% coverage probability were within the limit.

Pass[1] = The measurement result was within the limit. However, a portion of the expanded uncertainty of measurement at 95% exceeds the limit.

Fail[1] = The measurement result was out of the limit. However, a portion of the expanded uncertainty of measurement at 95% is within the limit.

Fail = The measurement result plus the expanded uncertainty with a 95% coverage probability were outside the limit.

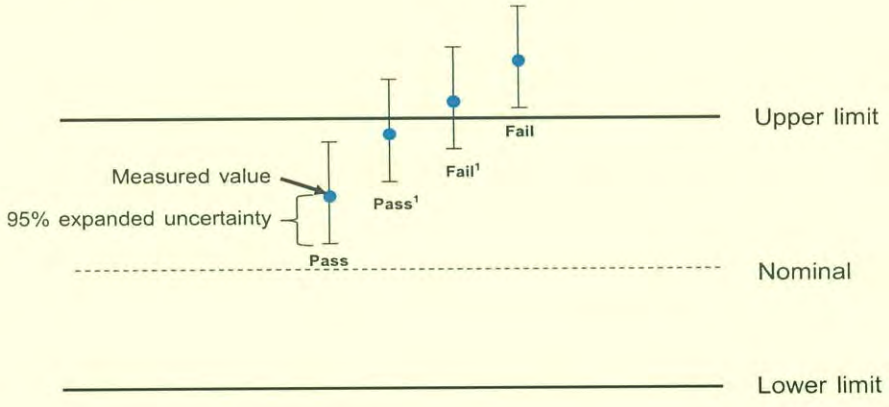

End of Certificate

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

ALS Laboratory Group (Thailand) Co., Ltd.
104 Phatthanakan 40, Phatthanakan Rd.,
Phatthanakan, Suan Luang, Bangkok 10250
T +66 2 760 3000 F +66 2 760 3197

Certificate of Calibration

Certificate No. C-070725-RYG_FS0144

Air Sampling Pump Detail

Equipment name	: Personal Air Sampling Pump	Equiment ID	: RYG_FS0144
Brand	: Gilian	Serial No.	: 20220731504
Model/Type	: GilAir Plus	Calibration Date	: 07-Jul-25
		Next calibration date	: 07-Oct-25

Reference Standard Low Flow Meter

Equipment name	: Air Flow Meter	Equiment ID	: RYG_FS0208
Brand	: MesaLabs	Serial No.	: 130027
Model/Type	: Defender 510-L	Calibration Date	: 27-Jan-25
		Due Date	: 26-Jan-26

Reference Standard High Flow Meter

Equipment name	: Air Flow Meter	Equiment ID	: BKK_FS0614
Brand	: MesaLabs	Serial No.	: 151114
Model/Type	: Defender 510-M	Calibration Date	: 9-Sep-24
		Due Date	: 9-Sep-25

Calibration Data

Air Sampling Pump setting (cc/min)	Reference Std. Flow Reading (cc/min)			Avg. (cc/min)	%Error acceptance	Acceptable range (cc/min)	Evaluation (Pass/ Fail)
	1	2	3				
Low Flow							
20	19.9	20.7	20.6	20.4	5%	19 - 21	Passed
50	51.8	51.3	51.7	51.6	5%	48 - 53	Passed
100	104.7	101.4	103.5	103.2	5%	95 - 105	Passed
200	206.8	207.7	204.4	206.3	5%	190 - 210	Passed
High Flow							
500	499.8	501.4	500.5	500.6	3%	485 - 515	Passed
1000	1000.5	1005.1	1001.8	1002.5	3%	970 - 1030	Passed
2000	1997.5	1995.2	1999.1	1997.3	3%	1940 - 2060	Passed
2500	2493.7	2486.4	2498.3	2492.8	3%	2425 - 2575	Passed

---------- END OF REPORT ----------

Calibrated By: ..... (Mr. Natchapon Thamklang)
RYG Field Services Scientist (1)

Approved By: ..... (Mr. Supot Salamteh)
Field Services Section Head

Issue date : 08-Jul-25

MULTI POINT CALIBRATION REPORT

CUSTOMER NAME : ALS Laboratory Group (Thailand) Co.Ltd. (สาขาระยอง)		
EQUIPMENT NAME : CO Analyzer		
MANUFACTURER : Teledyne - API	MODEL : T300	SERIAL NO : 1215
STANDARD GAS CONCENTRATION (PPM) : 808.9		CERTIFIED DATE : CC739972
CYLINDER PRESSURE (pslg) : 900		CERTIFIED DATE : Nov ,05 ,2020
CERTIFIED BY : AIRGAS SPECIALTY GASES		EXPIRED DATE : Nov ,05, 2028

CALIBRATION RESULTS

POINT NO	CALIBRATION RESULTS			
	IDEAL (PPM)	ACTUAL CO (PPM)	ERROR CO (PPM)	% ERROR CO
ZERO	0.00	0.008	0.008	-
1	40.00	40.015	0.015	0.038
2	80.00	79.445	-0.555	-0.694
3	199.20	200.083	0.883	0.443
4	400.60	397.683	-2.917	-0.728
5	808.90	808.538	-0.362	-0.045
AVERAGE (%)				0.390

REVIEW BY Thanita K.

APPROVED BY D. Thanyaporn

NEXT CAL. DATE 3 Jul 2026

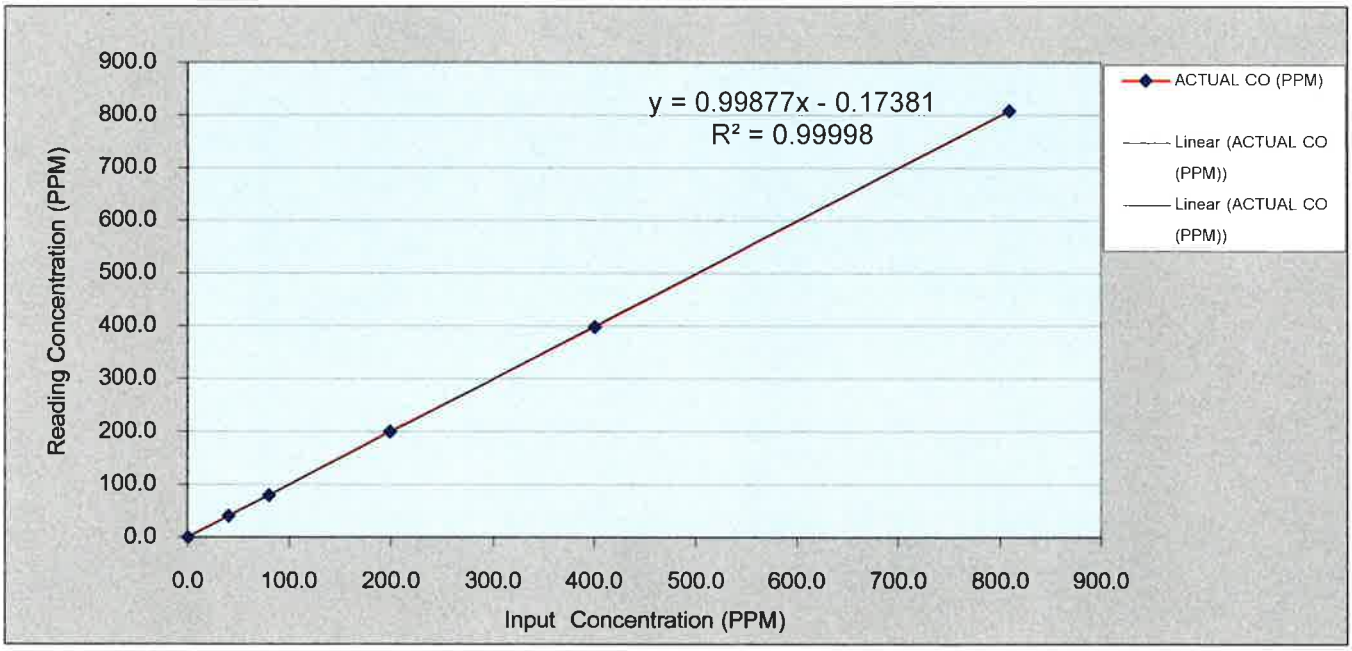

CALIBRATED BY : คุณธนาคม มหาอาจ	DATE : 3 กรกฎาคม 2568

ต้องการข้อมูลทางด้านเทคนิคเพิ่มเติม : คุณธนาคม มหาอาจ โทรศัพท์ : 02-515-8987

เลขที่ 388 ถนนรัชดาภิเษก แขวงจันทรเกษม เขตจตุจักร กรุงเทพฯ 10900 โทรศัพท์ : 0-2515-8999 โทรสาร : 0-2515-8988 E-Mail : Info@kinetics.co.th

KINETICS

บริษัท ไคเนติคส์ คอร์ปอเรชัน จำกัด

KINETICS CORPORATION LTD.

รายงานผลการซ่อมและปรับเทียบอุปกรณ์ตรวจวัดคุณภาพอากาศ

ลูกค้า / หน่วยงาน : ALS Laboratory Group (Thailand) Co.Ltd. (สาขาระยอง)
วันที่ : 3 กรกฎาคม 2568

รายชื่ออุปกรณ์ / เครื่องมือ : CO Analyzer
บริษัทผู้ผลิต : Teledyne API

รุ่นของอุปกรณ์ / เครื่องมือ : T300
หมายเลขอุปกรณ์ / เครื่องมือ : 1215

TEST VALUES				
	API MODEL T300		BEFORE	AFTER
1	RANGE	1 - 1000 PPM	100	100
2	STABILITY	≤ 1 PPM	0.015	0.099
3	CO MEASURE	2500 - 4800 mV	3210.3	3640.6
4	CO REFERENCE	2000 - 4800 mV	2660.3	3011.2
5	MR RATIO	1.1 - 1.3	1.220	1.218
6	PRESSEURE	25 - 35 in - Hg-A	29.1	29.0
7	SAMPLE FLOW	800 ± 10% cc/min	813	799
8	SAMPLE TEMP	48 ± 4 ^{0}C	45.2	44.9
9	BENCH TEMP	48 ± 2 ^{0}C	47.3	48.0
10	WHEEL TEMP	68 ± 2 ^{0}C	68.3	68.0
11	BOX TEMP	AMBIENT ± 5 ^{0}C	31.7	31.9
12	PHT DRIVE	250 - 4750 mV	4218.1	4206.5
13	CO SLOPE	1.0 ± 0.3	0.945	0.924
14	CO OFFSET	0.0 ± 0.3	0.007	0.007
15	CO READING (AMBIENT)	PPM	-0.455	0.333
17	VOLTAGE TEST	+5 V +12 V +15 V -15 V	5.22 / 12.18 / 16.72 / -15.29	5.22 / 12.18 / 16.72 / -15.29
18	ZERO GAS	0.00 PPM	0.080	0.008
19	SPAN GAS	40.00 PPM	41.440	40.015

หมายเหตุ

- ทำการเปลี่ยนวัสดุสิ้นเปลือง SS, Filter 1 ชิ้น, O-ring 2 ชิ้น , Spring 1 ชิ้น , Sample filter 47 mm. 1 ชิ้น
- ทำการ Calibrate Multi-Point

(คุณธนาคม มหาอาจ)

ลงนามเจ้าหน้าที่ (Signature)

ต้องการข้อมูลเพิ่มเติมทางด้านเทคนิค กรุณาติดต่อ : คุณธนาคม มหาอาจ โทรศัพท์ : 0-2515-8987
เลขที่ 388 ถนนรัชดาภิเษก แขวงจันทรเกษม เขตจตุจักร กรุงเทพฯ 10900 โทรศัพท์ : 0-2515-8999 โทรสาร : 0-2515-8988 E-Mail : Info@kinetics.co.th

KINETICS
Environmental science business Unit

Customer service report

ALS Laboratory Group (Thailand) Co., Ltd.

Manufacturer	Equipment	Model
Teledyne API	CO Analyzer	T300

S/N	Quotation
1215	-

● Checking Date ●

3/07/2025

● Problem

- Preventive Maintenance

B2

contact us

● Correlation working / Remark

1. ทำการเปลี่ยน Sintered Filter , O-ring , Spring
2. ทำการเปลี่ยน Sample Filter 47 mm
3. ทำการ Calibrate Multi - Point

● Repair parts ●

1. Sintered Filter 1 ชิ้น
2. O-ring 2 ชิ้น
3. Spring 1 ชิ้น
4. Filter 47 mm 1 ชิ้น

Technician / Engineer

Mr. Thanakom

CALIBRATION LABORATORY CO., LTD.
2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com

CLC Accredited ISO/IEC 17025

ANAB ANSI National Accreditation Board ACCREDITED ISO/IEC 17025 CALIBRATION AND DIMENSIONAL MEASUREMENT ACDM-2814

CERTIFICATE OF CALIBRATION

FOR

REVIEW BY Warakorn P.

APPROVED BY .....

NEXT CAL DATE 02/04/26

NOMENCLATURE	:	VACUUM GAUGE
MANUFACTURER	:	QUALITYWELL
MODEL / TYPE	:	N/A
SERIAL NO.	:	VG02[RYG_FS0333]
CLID. NO.	:	212300696
JOB CONTROL NO.	:	241002105107
CALIBRATION SERVICE	:	☑ IN-LABORATORY ☐ ON-SITE

CUSTOMER : ALS LABORATORY GROUP (THAILAND) CO., LTD.
104 PHATTHANAKAN 40, PHATTHANAKAN RD.,
KHWAENG PHATTHANAKAN, KHET SUAN LUANG, BANGKOK 10250, THAILAND

DATE OF RECEIVED : 02 October 2024 DATE OF ISSUED : 04 October 2024

The report of calibration shall not be reproduced except in full without approval of the Calibration Laboratory Co., Ltd.

Calibrated By : Sittipong Pimdee
Calibration Engineer

Approved By : Mongkol Yotsoontorn
Authorized Signatory
04 October 2024

This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to the International System of Units (SI)

Certificate No. Q24105107

@clccalibration

CALIBRATION LABORATORY CO., LTD.
2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com

CLC Accredited ISO/IEC 17025

ilac-MRA

ANAB ANSI National Accreditation Board ACCREDITED ISO/IEC 17025 CALIBRATION AND DIMENSIONAL MEASUREMENT ACDM-2814

REPORT OF CALIBRATION

FOR

NOMENCLATURE	:	**VACUUM GAUGE**
MANUFACTURER	:	**QUALITYWELL**
MODEL / TYPE	:	**N/A**
SERIAL NO.	:	**VG02[RYG_FS0333]**
DATE OF CALIBRATION	:	**03 October 2024**

ENVIRONMENT CONDITIONS :

Temperature : (23 ± 2) °C **Relative Humidity : (55 ± 10) %RH**

PROCEDURE USED :

This instrument was calibrated under procedure No. **CLC-CPPP-05** according to **DKD-R 6-1** as calibration guidelines.

The calibration was performed by direct measurement with Document Process Calibrator and Pressure Module which maintained by the Calibration Laboratory Co., Ltd.

REFERENCE STANDARD USED :

Document Process Calibrator, Fluke Model 741B S/N. 8295020 with Pressure Module Model 700PD5 S/N. 89404505.

TRACEABILITY :

The measurements are traceable to International System of Units (SI), through National Institute of Metrology (Thailand). Certificate No. MP-0040-24, Due Date 08 February 2025.

UNCERTAINTY :

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor of $k = 2$. It has been evaluated according to the "Calibration of Pressure Gauges (DKD-R 6-1)" which provides a level of confidence approximately 95%.

@clccalibration

CONDITION OF CALIBRATION ITEM : RECEIVED IN GOOD OPERATIONAL CONDITION

MEASUREMENT RESULTS : (X) without adjustment ( ) adjustment

The DUC was exercised by applying a known pressure from its zero to full scale 1 times. Then 2 series of known gauge pressure were applied. The STD reading were recorded and the means value were reported in the table below.

CALIBRATION DATA

CORRECTION OF PRESSURE

DUC Test point (inHg)	STD Reading (kPa)		Conversion to inHg		Correction (inHg)	
	Up	Down	Up	Down	Up	Down
-10.0	-33.62	-33.66	-9.93	-9.94	+0.07	+0.06
-20.0	-67.79	-67.82	-20.02	-20.03	-0.02	-0.03
-26.0	-88.41	-88.41	-26.11	-26.11	-0.11	-0.11
-27.0	-91.86	-91.90	-27.13	-27.14	-0.13	-0.14
-28.0	-95.35	-95.35	-28.16	-28.16	-0.16	-0.16

Uncertainty of measurement ± 0.08 inHg

Transmitting fluid : Air.

Technical Note. Conversion factor 1 kPa ; 0.2953003 inHg

Note. The Scope of Accredited ANAB Certificate No. ACDM-2814 Version 012 Page 43 of 67

This report is valid for the above stated instrument/s only.

End of Certificate

DKSH

NSC-TISI-TIS 17025
Calibration 0087

Certificate of Calibration

Equipment:	SPECTROPHOTOMETER	Certificate No.:	C06250108
Model:	DR6000	Issued Date:	18 March 2025
Serial No. (or ID.):	1627845 (RYG_EN0037)	Job No.:	WO-00064379
Manufacturer:	HACH	Page:	1 of 3
Condition:	In Condition		

Customer: ALS Laboratory Group (Thailand) Co.,Ltd. (Rayong Branch)
616/10 Moo 5 T.Maenam Khu,
A.Pluakdaeng, Rayong 21140, Thailand.

REVIEW BY Photchanas.
APPROVED BY D.
NEXT CAL. DATE 18/09/26

Environment Condition:	Temperature	24.4	°C	±	0.3	°C
	Humidity	60.8	%RH	±	3.5	%RH

Calibration Place: ALS Laboratory Group (Thailand) Co.,Ltd. (Rayong Branch)
(Wet Chemistry Lab)
616/10 Moo 5 T.Maenam Khu, A.Pluakdaeng, Rayong 21140, Thailand.

Calibration By: Mr.Preecha Phooarsai

Calibration Date: 18 March 2025

The Method used: In house method, CAL-WI-24, base on ASTM E 275-08 and ASTM E 387-04

Traceability: This certificate is traceable to the CRM maintained by National Institute of Standards and Technology (NIST) through Starna Scientific Limited.

The standard for Wavelength Certificate No. 111583 and 111584
The standard for Photometric Certificate No. 9114984 and 111588
The standard for Stray light Certificate No. 111586 and 111585
The standard for Spectral resolution Certificate No. 111587

(Mr. Preecha Phooarsai)
Person in charge

(Miss Kaewkan Suradech)
Authorized signatory

This certificate is issued the units of measurement according to the International System of Units (SI). It provides traceability of measurement to international or national standard or other recognized national standard laboratories.

The measurement uncertainty stated is the expanded uncertainty which is obtained from the standard uncertainty multiplied by the coverage factor (k=2) to provide a level of confidence of approximately 95%. It is determined in accordance with the Guide to Expression of Uncertainty in Measurement (GUM).

These results may be affected by deviations from specified conditions. The results relate only to the items tested, calibrated or sampled. The report shall not be reproduced except in full without approval of DKSH Technology Limited.

บริษัท ดีเคเอสเอช เทคโนโลยี จำกัด
DKSH Technology Limited
2533 ถนนสุขุมวิท แขวงบางจาก เขตพระโขนง กรุงเทพมหานคร 10260
2533 Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Phone: +66 2639 7000 Email: info.calibration@dksh.com Website: www.dksh.com/scientific-thailand

Calibration Results:

Without Adjustment

Wavelength Accuracy (nm), The spectral bandwidth of Std at 2 nm and UUC at 2 nm

Standard Wavelength	Unit Under Calibration	Correction	Uncertainty
418.61	418.5	0.11	0.13
536.66	536.7	-0.04	0.13
637.98	638.3	-0.32	0.13
748.48	748.8	-0.32	0.13
807.03	807.5	-0.47	0.13

Photometric Accuracy (Absorbance)

Wavelength	Standard absorbance	Unit Under Calibration	Correction	Uncertainty
420 nm	0.0000	0.000	0.0000	0.0045
	0.2930	0.291	0.0020	0.0045
	0.5168	0.518	-0.0012	0.0045
	1.0298	1.031	-0.0012	0.0045
440 nm	0.0000	0.000	0.0000	0.0045
	0.2867	0.285	0.0017	0.0045
	0.5073	0.508	-0.0007	0.0045
	1.0083	1.009	-0.0007	0.0045
465 nm	0.0000	0.000	0.0000	0.0045
	0.2516	0.250	0.0016	0.0045
	0.4595	0.461	-0.0015	0.0045
	0.9334	0.935	-0.0016	0.0045
546.1 nm	0.0000	0.000	0.0000	0.0045
	0.2461	0.246	0.0001	0.0045
	0.4652	0.466	-0.0008	0.0045
	0.9468	0.948	-0.0012	0.0045
590 nm	0.0000	0.000	0.0000	0.0045
	0.2594	0.259	0.0004	0.0045
	0.5040	0.505	-0.0010	0.0045
	1.0032	1.004	-0.0008	0.0045
635 nm	0.0000	0.000	0.0000	0.0045
	0.2579	0.258	-0.0001	0.0045
	0.4971	0.497	0.0001	0.0045
	0.9720	0.973	-0.0010	0.0045

บริษัท ดีเคเอสเอช เทคโนโลยี จำกัด
DKSH Technology Limited
2533 ถนนสุขุมวิท แขวงบางจาก เขตพระโขนง กรุงเทพมหานคร 10260
2533 Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Phone: +66 2639 7000 Email: info.calibration@dksh.com Website: www.dksh.com/scientific-thailand

Calibration Results:

Without Adjustment

Photometric Accuracy (Absorbance)

Wavelength	Standard absorbance	Unit Under Calibration	Correction	Uncertainty
235 nm	0.0000	0.000	0.0000	0.0080
	0.7355	0.738	-0.0025	0.0080
257 nm	0.0000	0.000	0.0000	0.0080
	0.8574	0.857	0.0004	0.0080
313 nm	0.0000	0.000	0.0000	0.0080
	0.2864	0.290	-0.0036	0.0080
350 nm	0.0000	0.000	0.0000	0.0080
	0.6374	0.637	0.0004	0.0080

Stray light *

Standard: cut-off	UUC: Wavelength (nm)	UUC: Transmission (%T)	Absorbance (A)
260.62 +/- 0.11 nm	260.6	1.7	1.770
391.44 +/- 0.11 nm	391.4	1.4	1.854

Spectral Resolution *

Nominal Concentration 0.02 % v/v	Peak	Trough	Ratio	SBW
Standard Wavelength (nm)	268.66	266.69	1.38	2.00
UUC: Wavelength (nm)	268.2	266.2		
Std Absorbance (A)	0.4566	0.2780		
UUC: Absorbance (A)	0.413	0.299		

* Calibration Marked " Not TISI Accredited " in this Certificate have been included for completeness.

The End of Certificate

บริษัท ดีเคเอสเอช เทคโนโลยี จำกัด
DKSH Technology Limited
2533 ถนนสุขุมวิท แขวงบางจาก เขตพระโขนง กรุงเทพมหานคร 10260
2533 Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Phone: +66 2639 7000 Email: info.calibration@dksh.com Website: www.dksh.com/scientific-thailand

ใบตรวจสอบสภาพเครื่องวัดสิ่งแวดล้อม

เลขที่ใบงาน: WO-00064379

ชนิดเครื่องมือ: SPECTROPHOTOMETER รุ่น: DR6000 หมายเลขเครื่อง: 1627845

ตรวจสอบ (รับ) 18 Mar 2025		รายการตรวจเช็ค	ตรวจสอบ (ส่ง) 18 Mar 2025		หมายเหตุ
ปกติ	ไม่ปกติ		ปกติ	ไม่ปกติ	
		General			
☑	☐	1. ความสมบูรณ์เครื่อง	☑	☐	
☑	☐	2. ความสะอาด (ช่องใส่ตัวอย่าง, ภายใน-นอกเครื่อง)	☑	☐	
☑	☐	3. สวิทช์ ปิด – เปิด เครื่อง (On-Off Swicth)	☑	☐	
☑	☐	4. ปุ่มกด (Keypad)	☑	☐	
☑	☐	5. หน้าจอ (Display, Screen Contrast)	☑	☐	
		Spectrophotometer			
☐	☐	6. แรงดันไฟฟ้า (Battery Backup) >= 2.5 VDC	☐	☐	
☐	☐	7. ตัวหมุนเลือกความยาวคลื่น (Wavelength Control)	☐	☐	
☑	☐	8. ความยาวคลื่น (Wavelength Check)	☑	☐	*
☑	☐	9. แหล่งกำเนิดแสง (UV < 3,000 hour)	☑	☐	13.5 Hours
☑	☐	10. แหล่งกำเนิดแสง (Visible < 5,000 hour)	☑	☐	893.0 Hours
☑	☐	11. ช่องวัดหลายตัวอย่าง (Carousel Module)	☑	☐	
		pH Meter and Conductivity Meter			
☐	☐	12. อิเล็คโทรด (Electrode and Connection Cable)	☐	☐	
☐	☐	13. ระดับสารละลายใน Electrode (Level KCl)	☐	☐	
☐	☐	14. ฝาปิดกันปลาย Electrode (Dust Protection Hood)	☐	☐	
☐	☐	15. ขาจับอิเล็คโทรด (Stand)	☐	☐	
		Turbidimeter			
☐	☐	16. ค่าความขุ่นที่ต่ำสุด (No Sample)	☐	☐	
☐	☐	17. ระดับการส่องสว่างของแสง (>= 2.5 ไม่เกิน 3.0)	☐	☐	
		Automatic titrator			
☐	☐	18. สภาพ Piston Burettes	☐	☐	
☐	☐	19. Function Rinsing and Dosing	☐	☐	
☐	☐	20. ระบบท่อสายยางและอุปกรณ์ประกอบ	☐	☐	

เพิ่มเติม/ข้อแนะนำ : * 656.1nm = 656.1nm

* 486.0nm = 485.7nm

Mr.Preecha Phooarsai

Service Engineer

บริษัท ดีเคเอสเอช เทคโนโลยี จำกัด
DKSH Technology Limited
2533 ถนนสุขุมวิท แขวงบางจาก เขตพระโขนง กรุงเทพมหานคร 10260
2533 Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Phone: +66 2639 7000 Email: info.calibration@dksh.com Website: www.dksh.com/scientific-thailand

Accredited by

NSC-TISI-TIS 17025
Calibration 0426

Calibration certificate

Calibration Certificate No. 25BKL0003

Object	Electronic non-automatic weighing instrument
Manufacturer	Sartorius
Type	MSU224S-100-DU
Serial | QM Ident. no.	31709552 | RYG_EN0003
Customer	ALS Laboratory Group (Thailand) Co.,Ltd. (Rayong Branch) 616/10 Moo 5 T.Maenam Khu, A.Pluak Daeng, Rayong 21140, Thailand.
Order no.	2230
Number of pages	4
Date of calibration	20 Feb 2025

This calibration certificate documents the traceability to national standards.

Uncertainties of measurements are taken into account when only statements of compliance are made.

This certificate was prepared by Sartorius Corporation in accordance to the current ISO/IEC 17025:2017 standard and Sartorius Work Instruction (Method) SOP WI 08.

This certificate relate and apply this equipment only.

REVIEW BY ..... Thanitak.

APPROVED BY..... D. Chumon.

NEXT CAL DATE.....20/02/26.....

This calibration certificate may not be reproduced other than in full except with the permission of NSC-TISI-TIS-17025 and the issuing laboratory. Calibration certificates without signature are not valid.

The user is obliged to have the object recalibrated at appropriate intervals.

Date	Approval of the Calibration Certificate	Person in charge
06 Mar 2025	Mr. Chonchai Inthana	Kachen Lalee

Calibration object

Single range instrument

Model	MSU224S-100-DU
Serial Number	31709552
QM Ident. no | Inventory no.	RYG_EN0003 | ---

Maximum capacity (Max. load)	220.0000 g
Measured range	220.0000 g
Scale interval	0.0001 g

Place of calibration

Address	According to page 1
Department | Cost center	Laboratory Department. | ---
Building | Floor	--- | 1st Floor.
Room	Balance Room.
Maximum temperature variation at place of calibration	5 K

Calibration procedure

EURAMET cg-18, V4.0 - Guidelines on the Calibration of Non-Automatic Weighing Instruments

Test equipment

Test equipment type	Test equipment ID	Valid until
Thermometer	MHB-382SD s/nB011342 Traceable to SI unit through DKSH	21 Aug 2025
Test weight set OIML R111 E2	Certificate No.M2308197S ,E2(Traceable to SI unit through TCS)	23 Aug 2025

Adjustment Status

The measuring device was internally adjusted before the calibration.

Environmental and measuring conditions

Date of calibration	20 Feb 2025
Temperature at place of calibration | Temp. diff. $T_{weights}$ - T_{place}	24.7 °C | 0.3 K
Measuring conditions	The installation site is suitable. The device was levelled. Balance was loaded up to Max before test.
Comments	Humidity 62.3 %RH.

Measurement results | Measurement uncertainties

Repeatability

Test load (nominal): 10 g | 200 g

	10 g	200 g
1	10.0000 g	200.0000 g
2	10.0000 g	200.0001 g
3	9.9999 g	200.0000 g
4	10.0000 g	200.0000 g
5	10.0000 g	200.0001 g
6	9.9999 g	200.0000 g
7	10.0000 g	200.0000 g
8	10.0000 g	200.0000 g
9	10.0000 g	200.0000 g
10	10.0000 g	200.0001 g
	s = 0.00004 g	s = 0.00005 g

Eccentricity

Test load (nominal):	**100 g**
Center	100.0000 g
Front left	100.0000 g
Back left	100.0001 g
Back right	99.9999 g
Front right	99.9999 g
Maximum deviation from centric loading indication $\lvert\Delta I_{ecc}\rvert_{max}$ = 0.0001 g	

Error of indication

Testload L	Indication I	Error E	Expansion factor k	Uncertainty $U(E)$	Uncertainty relative $U_{rel}(E)$
0.0100 g	0.0100 g	0.0000 g	2.00	0.00012 g	1.2 %
0.1000 g	0.1000 g	0.0000 g	2.00	0.00013 g	0.13 %
0.5000 g	0.5000 g	0.0000 g	2.00	0.00013 g	0.026 %
1.0000 g	1.0000 g	0.0000 g	2.00	0.00013 g	0.013 %
5.0000 g	5.0000 g	0.0000 g	2.00	0.00013 g	0.0026 %
10.0000 g	10.0000 g	0.0000 g	2.00	0.00013 g	0.0013 %
20.0000 g	20.0000 g	0.0000 g	2.00	0.00014 g	0.00068 %
50.0000 g	50.0000 g	0.0000 g	2.00	0.00015 g	0.00029 %
100.0000 g	100.0001 g	0.0001 g	2.00	0.00018 g	0.00018 %
200.0000 g	200.0000 g	0.0000 g	2.00	0.00028 g	0.00014 %
220.0000 g	220.0000 g	0.0000 g	2.00	0.00032 g	0.00015 %
Maximum error of indication		$\lvert E\rvert_{max}$ = 0.0001 g			

$U_{rel}(E)$ is the quotient of $U(E)$ and test load L. The uncertainty of measurement $U(E)$ is valid only if error E is considered. You will find reference notes on the uncertainty of measurement in use under: Appendix to the calibration certificate | Interpretation of measurement results.
Reference note: The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the documented Expansion factor, determined in accordance with the European Calibration Guideline EURAMET cg-18, V4.0. There is a 95 % probability that the value of the measurand will be in the assigned value range.

End of calibration certificate

Uncertainty of measurement in use

Device adjusted before measurement	Yes
Temperature deviation considered	1.5 K (isoCAL active)
Temperature coefficient considered	$1 \cdot 10^{-6}$/K
Uncertainty of the weighing result $U_{gl}(W)$	**$U_{gl}(W) = 0.00013\ g + 3.42 \cdot 10^{-6} \cdot R$**

Reference note: The current uncertainty of measurement is calculated by entering of the reading *R* into this formula. In relation to this, there is no need for a correction of the indication error. The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied with an Expansion factor of 2, determined in accordance with the European Calibration Guideline EURAMET cg-18, V4.0. There is a 95 % probability that the value of the measurand will be in the assigned value range.

Indication in % from max load	Net indication *R*	Uncertainty $U_{gl}(W)$	Uncertainty relative $U_{gl}(W)_{rel}$
1 %	2.2000 g	0.00014 g	0.0063 %
25 %	55.0000 g	0.00032 g	0.00058 %
50 %	110.0000 g	0.00051 g	0.00046 %
75 %	165.0000 g	0.00069 g	0.00042 %
100 %	220.0000 g	0.00088 g	0.00040 %

Graphic realization of the relative uncertainty of measurement | process accuracy

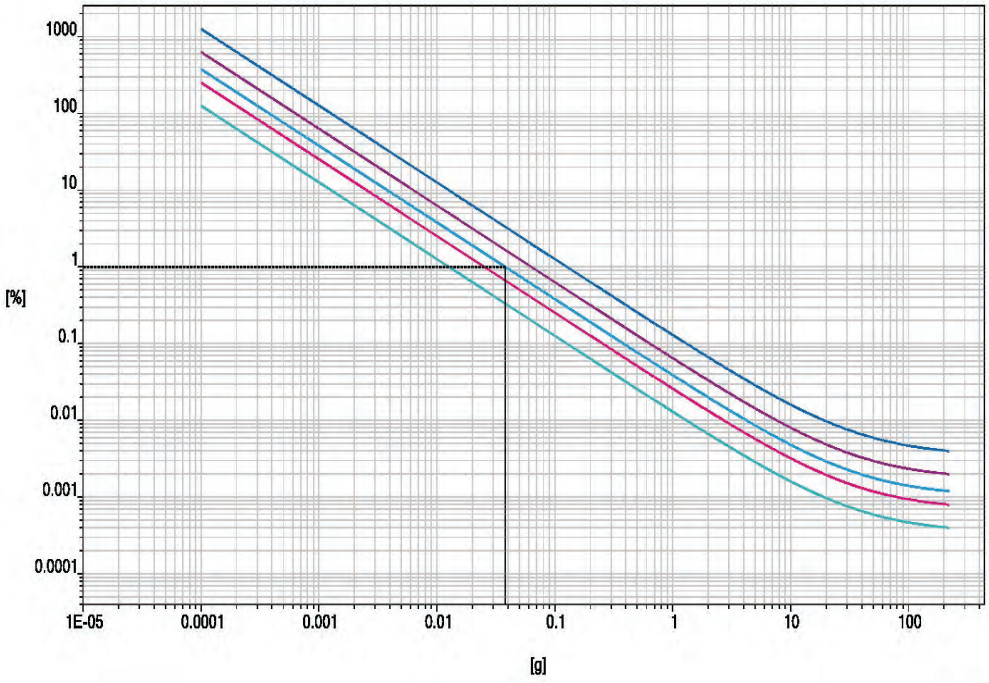

Safety factor

10	
5	
3	
2	
1	

Displayed example

Process accuracy	1.00 %
Safety factor	3
Minimum sample weight	0.0380 g

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7/139 MOO 13, SOI SUNTINAKORN 11 TAMBON BANG KAEO,
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL: (66)0-2116-5860-1 FAX: (66)0-2116-7140

Certificate of Calibration

Customer

Certificate No : 25-AFM-208

Name : ALS Laboratory Group Thailand Co., Ltd.

Request No : Req-2025-1986

Address : 104 Soi Phatthanakan 40, Phatthanakan Road, Suan Luang, Bangkok 10250

Unit Under Calibration Details

Measurement Item : Air Flow Meter

Manufacturer : Mesa Labs

Sensor Model : -

Model : 200-510M

Sensor Serial Number : -

Serial Number : 151114

Instrument Status : Used

ID : BKK_FS0614

Location of Calibration : LAB 4 AIR VELOCITY METER

Calibration Environment and Details

REVIEW BY ..... Narakorn P.

APPROVED BY.....

NEXT CAL DATE..... 09/09/26

Temperature : 23 °C ± 3 °C

Humidity : 55 %RH ± 20 %RH

Barometric Pressure : 1013 hPa ± 10 hPa

Received Date : 3 September 2025

Calibration Date : 10 September 2025

Calibration Procedure : In-house method CP-AFM-01 by Comparison technique with Standard Primary Flow Calibrator

Reference Standard	Model	Serial Number	Traceble	Due Calibration
Air Flow Meter	Gilibrator 3 Low flow	18501010006	Sensidyne	5 May 2026
Air Flow Meter	Gilibrator 3 Standard flow	19031011003	Sensidyne	6 May 2026
Temperature meter	GT 11	08000057	Qreborn	15 October 2025
Pressure meter	CPG2400	41000KDU/651882	TPA	21 October 2025

Traceability :

This Certificate is traceable to SI Unit through Sensidyne A2LA Accreditation No. 3943.01 and MIT NSC-TISI-TIS Accreditation No. 0052

Note :

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor k = 2, providing a level of confidence approximately 95 %.

Calibration By :

Mr. Noppadon Luangart

Service Calibration Engineer

Approved By :

Mr. Pacit Mathavorn

Calibration Engineer Supervisor

Issue Date : 10 September 2025

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7/139 MOO 13, SOI SUNTINAKORN 11 TAMBON BANG KAEO,
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL: (66)0-2116-5860-1 FAX: (66)0-2116-7140

Certificate No : 25-AFM-208

Request No : Req-2025-1986

Result of Calibration : Without Adjustment

STD Reading			UUC Readinng			Error	Uncertainty		
Temperature (°C)	Pressure (kPa)	Flow (cc/min)	Temperature (°C)	Pressure (kPa)	Flow (cc/min)	(cc/min)	(cc/min)	(°C)	(kPa)
25.5	100.98	100	-	-	100.02	0.0	3.6	1.0	0.50
25.7	100.97	503	-	-	500.81	-2.2	9.5	1.0	0.50
25.8	100.89	1003	-	-	1000.4	-3	19	1.0	0.50
26.1	100.88	2000	-	-	2001.9	2	38	1.0	0.50
26.5	100.85	3014	-	-	3002.2	-12	57	1.0	0.50
26.7	100.81	4027	-	-	4000.9	-26	76	1.0	0.50
27.0	100.74	5048	-	-	5001.8	-46	95	1.0	0.50

Note STD : Standard UUC : Unit Under Calibration

- UUC Reference Condition : At atmospheric pressure and room temperature condition, Air
- Flow Rate was corrected for non-standard operating condition by using equation :

$$Qmeas = \mathrm{Qref}\, x \frac{\mathrm{Pref}}{\mathrm{Pmeas}} x \frac{\mathrm{Tmeas}}{\mathrm{Tref}}$$

where Q = Flow Rate P = Absolute Pressure T = Absolute Temperature
meas = Measurement Condition ref = Standard Condition

* Indicates non accredited

End of Certificate

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7/139 MOO 13, SOI SUNTINAKORN 11 TAMBON BANG KAEO,
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL: (66)0-2116-5860-1 FAX: (66)0-2116-7140

Certificate of Calibration

Customer

Certificate No : 24-AFM-177

Name : ALS Laboratory Group Thailand Co., Ltd.

Request No : Req-2024-1862

Address : 104 Soi Phatthanakan 40, Phatthanakan Road, Suan Luang, Bangkok 10250

Unit Under Calibration Details

Measurement Item : Air Flow Meter

Manufacturer : Bios

Accuracy : 1% of Reading

Model : Defender 510-L

Sensor Model : -

Serial Number : 130026

Sensor Serial Number : -

ID : BKK_FS0619

Instrument Status : Used

Location of Calibration : LAB 4 AIR VELOCITY METER

REVIEW BY Marakorn P

APPROVED BY

NEXT CAL. DATE 9/9/26

Calibration Environment and Details

Temperature : 23 °C ± 3 °C

Humidity : 55 %RH ± 20 %RH

Barometric Pressure : 1013 hPa ± 10 hPa

Received Date : 22 August 2024

Calibration Date : 9 September 2024

Calibration Procedure : In-house method CP-AFM-01 by Comparison technique with Standard Primary Flow Calibrator

Reference Standard	Model	Serial Number	Traceble	Due Calibration
Air Flow Meter	Gilibrator 3 Low flow	18501010006	Sensidyne	6 August 2025
Air Flow Meter	Gilibrator 3 Standard flow	19031011003	Sensidyne	2 August 2025
Temperature meter	GT 11	08000057	Qreborn	1 March 2025
Pressure meter	CPG2400	41000KDU/651882	TPA	9 November 2024

Traceability :

This Certificate is traceable to SI Unit through Sensidyne A2LA Accreditation No. 3943.01

Note :

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor $k = 2$, providing a level of confidence approximately 95 %.

Calibration By :

Mr. Noppadon Luangart

Service Calibration Engineer

Approved By :

Mr. Pacit Mathavorn

Calibration Engineer Supervisor

Issue Date : 9 September 2024

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7/139 MOO 13, SOI SUNTINAKORN 11 TAMBON BANG KAEO,
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL: (66)0-2116-5860-1 FAX: (66)0-2116-7140

Certificate No : 24-AFM-177

Request No : Req-2024-1862

Result of Calibration : Without Adjustment

Temperature (°C)	Pressure (kPa)	STD (cc/min)	UUC (cc/min)	Error (cc/min)	Uncertainty (cc/min)	MPE (cc/min)	Result
24.70	100.92	20	20.192	0.2	1.3	0.2	N/A
24.70	100.90	100	99.923	-0.1	2.8	1.0	N/A
24.70	100.94	201	200.7	-0.3	5.6	2.0	N/A
24.70	100.97	298	300.1	2.1	8.4	3.0	N/A
24.70	100.99	403	399.1	-4	11	4.0	N/A
24.80	101.05	482	477.6	-4.4	6.9	4.8	N/A

Note STD : Standard UUC : Unit Under Calibration

- UUC Reference Condition : At atmospheric pressure and room temperature condition
- Flow Rate was corrected for non-standard operating condition by using equation :

$$Q_{meas} = Q_{ref} \times \frac{P_{ref}}{P_{ref}} \times \frac{T_{meas}}{T_{ref}}$$

where Q = Flow Rate P = Absolute Pressure T = Absolute Temperature
Meas = Measurement Condition ref = Standard Condition

* Indicates non accredited

MPE = Maximum Permissible Error (Specified in Manufacturer's Specifications)

N/A = Not Aavailable, Customer does not require a statement of conformity.

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7/139 MOO 13, SOI SUNTINAKORN 11 TAMBON BANG KAEO,
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL: (66)0-2116-5860-1 FAX: (66)0-2116-7140

Certificate No : 24-AFM-177

Request No : Req-2024-1862

Decision Rule for Statements of Conformity

The standard decision rule employed for the statements of conformity to each calibration result will be applied using ILAC-G8:09/2019; Guidelines on the Reporting of Compliance with Specification as following Fig. and statements

Pass = The measurement result plus the expanded uncertainty with a 95% coverage probability were within the limit.

Pass[1] = The measurement result was within the limit. However, a portion of the expanded uncertainty of measurement at 95% exceeds the limit.

Fail[1] = The measurement result was out of the limit. However, a portion of the expanded uncertainty of measurement at 95% is within the limit.

Fail = The measurement result plus the expanded uncertainty with a 95% coverage probability were outside the limit.

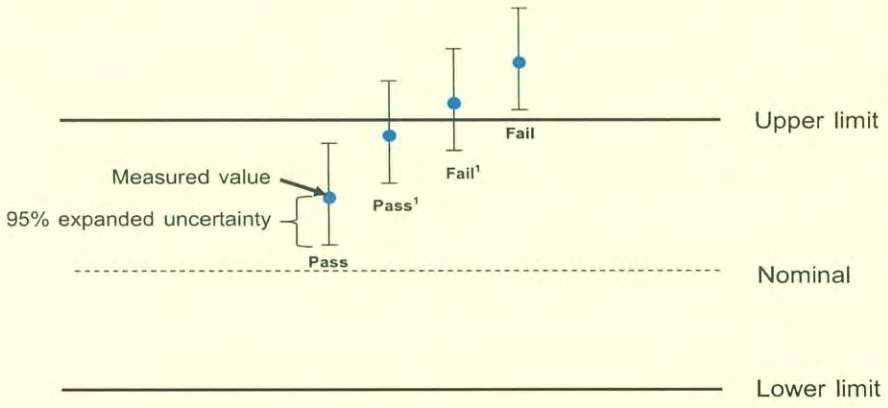

End of Certificate

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7/139 MOO 13, SOI SUNTINAKORN 11 TAMBON BANG KAEO,
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL.: (66)0-2116-5860-1 FAX: (66)0-2116-7140

Certificate of Calibration

Customer

Certificate No : 25-AFM-207

Name : ALS Laboratory Group Thailand Co., Ltd.

Request No : Req-2025-1987

Address : 104 Soi Phatthanakan 40, Phatthanakan Road, Suan Luang, Bangkok 10250

Unit Under Calibration Details

Measurement Item : Air Flow Meter

Manufacturer : Mesa Labs

Sensor Model : -

Model : 200-510L

Sensor Serial Number : -

Serial Number : 130026

Instrument Status : Used

ID : BKK_FS0619

Location of Calibration : LAB 4 AIR VELOCITY METER

REVIEW BY ..... Narakorn P. .....

APPROVED BY .....

NEXT CAL DATE..... 09/09/26 .....

Calibration Environment and Details

Temperature : 23 °C ± 3 °C

Humidity : 55 %RH ± 20 %RH

Barometric Pressure : 1013 hPa ± 10 hPa

Received Date : 3 September 2025

Calibration Date : 10 September 2025

Calibration Procedure : In-house method CP-AFM-01 by Comparison technique with Standard Primary Flow Calibrator

Reference Standard	Model	Serial Number	Traceble	Due Calibration
Air Flow Meter	Gilibrator 3 Low flow	18501010006	Sensidyne	5 May 2026
Air Flow Meter	Gilibrator 3 Standard flow	19031011003	Sensidyne	6 May 2026
Temperature meter	GT 11	08000057	Qreborn	15 October 2025
Pressure meter	CPG2400	41000KDU/651882	TPA	21 October 2025

Traceability :

This Certificate is traceable to SI Unit through Sensidyne A2LA Accreditation No. 3943.01 and MIT NSC-TISI-TIS Accreditation No. 0052

Note :

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor $k = 2$, providing a level of confidence approximately 95 %.

Calibration By :

Mr. Noppadon Luangart

Service Calibration Engineer

Approved By :

Mr. Pacit Mathavorn

Calibration Engineer Supervisor

Issue Date : 10 September 2025

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7/139 MOO 13, SOI SUNTINAKORN 11 TAMBON BANG KAEO,
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL.: (66)0-2116-5860-1 FAX: (66)0-2116-7140

Certificate No : 25-AFM-207

Request No : Req-2025-1987

Result of Calibration : Without Adjustment

STD Reading			UUC Readinng			Error	Uncertainty		
Temperature (°C)	Pressure (kPa)	Flow (cc/min)	Temperature (°C)	Pressure (kPa)	Flow (cc/min)	(cc/min)	(cc/min)	(°C)	(kPa)
25.5	100.98	20	-	-	20.042	0.0	1.6	1.0	0.50
25.5	100.90	50	-	-	49.921	-0.1	4.0	1.0	0.50
25.5	100.91	100	-	-	100.09	0.1	3.6	1.0	0.50
25.4	100.86	150	-	-	150.34	0.3	5.4	1.0	0.50
25.6	100.93	199	-	-	200.17	1.2	7.2	1.0	0.50
25.6	100.95	301	-	-	300.05	-1	11	1.0	0.50
25.7	100.96	402	-	-	401.03	-1	14	1.0	0.50
25.7	100.95	503	-	-	500.26	-3	10	1.0	0.50

Note STD : Standard UUC : Unit Under Calibration

- UUC Reference Condition : At atmospheric pressure and room temperature condition, Air
- Flow Rate was corrected for non-standard operating condition by using equation :

$$Qmeas = \mathrm{Qref}\, x \frac{\mathrm{Pref}}{\mathrm{Pmeas}} x \frac{\mathrm{Tmeas}}{\mathrm{Tref}}$$

where Q = Flow Rate P = Absolute Pressure T = Absolute Temperature
meas = Measurement Condition ref = Standard Condition

* Indicates non accredited

End of Certificate

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

Accredited by

NSC-TISI-TIS 17025
Calibration 0426

Calibration certificate

Calibration Certificate No. 25BKL0006

Object	Electronic non-automatic weighing instrument
Manufacturer	Sartorius
Type	MSE125P-100-DU
Serial | QM Ident. no.	33108993 | RYG_EN0004
Customer	ALS Laboratory Group (Thailand) Co.,Ltd. (Rayong Branch) 616/10 Moo 5 T.Maenam Khu, A.Pluak Daeng, Rayong 21140, Thailand.
Order no.	2230
Number of pages	4
Date of calibration	20 Feb 2025

This calibration certificate documents the traceability to national standards.

Uncertainties of measurements are taken into account when only statements of compliance are made.

This certificate was prepared by Sartorius Corporation in accordance to the current ISO/IEC 17025:2017 standard and Sartorius Work Instruction (Method) SOP WI 08.

This certificate relate and apply this equipment only.

REVIEW BY ThanitaK.

APPROVED BY D.Khunou.

NEXT CAL DATE 20/02/26

This calibration certificate may not be reproduced other than in full except with the permission of NSC-TISI-TIS-17025 and the issuing laboratory. Calibration certificates without signature are not valid.

The user is obliged to have the object recalibrated at appropriate intervals.

Date	Approval of the Calibration Certificate	Person in charge
06 Mar 2025	Mr. Chonchai Inthana	Kachen Lalee

Calibration object

Multi interval instrument

Model	MSE125P-100-DU	
Serial Number	33108993	
QM Ident. no | Inventory no.	RYG_EN0004 | ---	
Range	1	2
Maximum capacity (Max. load)	60.00000 g	120.0000 g
Measured range	60.00000 g	120.0000 g
Scale interval	0.00001 g	0.0001 g

Place of calibration

Address	According to page 1
Department | Cost center	Laboratory Department. | ---
Building | Floor	--- | 1st Floor.
Room	Balance Room.
Maximum temperature variation at place of calibration	5 K

Calibration procedure

EURAMET cg-18, V4.0 - Guidelines on the Calibration of Non-Automatic Weighing Instruments

Test equipment

Test equipment type	Test equipment ID	Valid until
Thermometer	MHB-382SD s/nB011342 Traceable to SI unit through DKSH	21 Aug 2025
Test weight set OIML R111 E2	Certificate No.M2308197S ,E2(Traceable to SI unit through TCS)	23 Aug 2025

Adjustment Status

The measuring device was internally adjusted before the calibration.

Environmental and measuring conditions

Date of calibration	20 Feb 2025
Temperature at place of calibration | Temp. diff. $T_{weights}$ - T_{place}	24.2 °C | 0.3 K
Measuring conditions	The installation site is suitable. The device was levelled. Balance was loaded up to Max before test.
Comments	Humidity 62.5 %RH.

Measurement results | Measurement uncertainties

Repeatability

Test load (nominal): 50 g | 100 g

	50 g	100 g
1	50.00002 g	100.0000 g
2	50.00001 g	100.0000 g
3	50.00003 g	100.0000 g
4	50.00002 g	100.0000 g
5	50.00001 g	100.0000 g
6	50.00002 g	99.9999 g
7	50.00002 g	100.0000 g
8	50.00001 g	100.0000 g
9	50.00001 g	100.0000 g
10	50.00002 g	100.0000 g
	s = 0.000007 g	s = 0.00003 g

Eccentricity

Test load (nominal):	**50 g**
Center	50.00002 g
Front left	50.00000 g
Back left	50.00000 g
Back right	50.00001 g
Front right	50.00003 g
Maximum deviation from centric loading indication $\lvert\Delta I_{ecc}\rvert_{max}$ = 0.00002 g	

Error of indication

Testload L	Indication I	Error E	Expansion factor k	Uncertainty $U(E)$	Uncertainty relative $U_{rel}(E)$
0.01000 g	0.01000 g	0.00000 g	2.00	0.000024 g	0.24 %
0.10000 g	0.10000 g	0.00000 g	2.00	0.000037 g	0.037 %
1.00000 g	1.00000 g	0.00000 g	2.00	0.000037 g	0.0037 %
5.00002 g	5.00002 g	0.00000 g	2.00	0.000050 g	0.0010 %
20.00002 g	20.00002 g	0.00000 g	2.00	0.000069 g	0.00034 %
55.00004 g	55.00003 g	-0.00001 g	2.00	0.00017 g	0.00031 %
70.0000 g	70.0000 g	0.0000 g	2.00	0.00017 g	0.00024 %
80.0001 g	80.0001 g	0.0000 g	2.00	0.00018 g	0.00023 %
100.0000 g	100.0000 g	0.0000 g	2.00	0.00017 g	0.00017 %
110.0000 g	110.0000 g	0.0000 g	2.00	0.00028 g	0.00025 %
120.0000 g	119.9999 g	-0.0001 g	2.00	0.00028 g	0.00023 %
Maximum error of indication		$\lvert E\rvert_{max}$ = 0.00010 g			

$U_{rel}(E)$ is the quotient of $U(E)$ and test load L. The uncertainty of measurement $U(E)$ is valid only if error E is considered. You will find reference notes on the uncertainty of measurement in use under: Appendix to the calibration certificate | Interpretation of measurement results.
Reference note: The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the documented Expansion factor, determined in accordance with the European Calibration Guideline EURAMET cg-18, V4.0. There is a 95 % probability that the value of the measurand will be in the assigned value range.

End of calibration certificate

Uncertainty of measurement in use

Device adjusted before measurement	Yes
Temperature deviation considered	1.5 K (isoCAL active)
Temperature coefficient considered	$1 \cdot 10^{-6}$/K

Uncertainty of the weighing result $U_{gl}(W)$

Partial weighing range 1 | 0.00000 g...60.00000 g	$U_{gl}(W) = 0.000016\ g + 6.61 \cdot 10^{-6} \cdot R$
Partial weighing range 2 | 60.00000 g...120.0000 g	$U_{gl}(W) = 0.000086\ g + 6.19 \cdot 10^{-6} \cdot R$

Reference note: The current uncertainty of measurement is calculated by entering of the reading *R* into this formula. In relation to this, there is no need for a correction of the indication error. The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied with an Expansion factor of 2, determined in accordance with the European Calibration Guideline EURAMET cg-18, V4.0. There is a 95 % probability that the value of the measurand will be in the assigned value range.

Indication in % from Max1	Net indication *R*	Uncertainty $U_{gl}(W)$	Uncertainty relative $U_{gl}(W)_{rel}$
1 %	0.60000 g	0.000020 g	0.0033 %
25 %	15.00000 g	0.00012 g	0.00077 %
50 %	30.00000 g	0.00021 g	0.00071 %
75 %	45.00000 g	0.00031 g	0.00070 %
100 %	60.00000 g	0.00041 g	0.00069 %

Graphic realization of the relative uncertainty of measurement | process accuracy

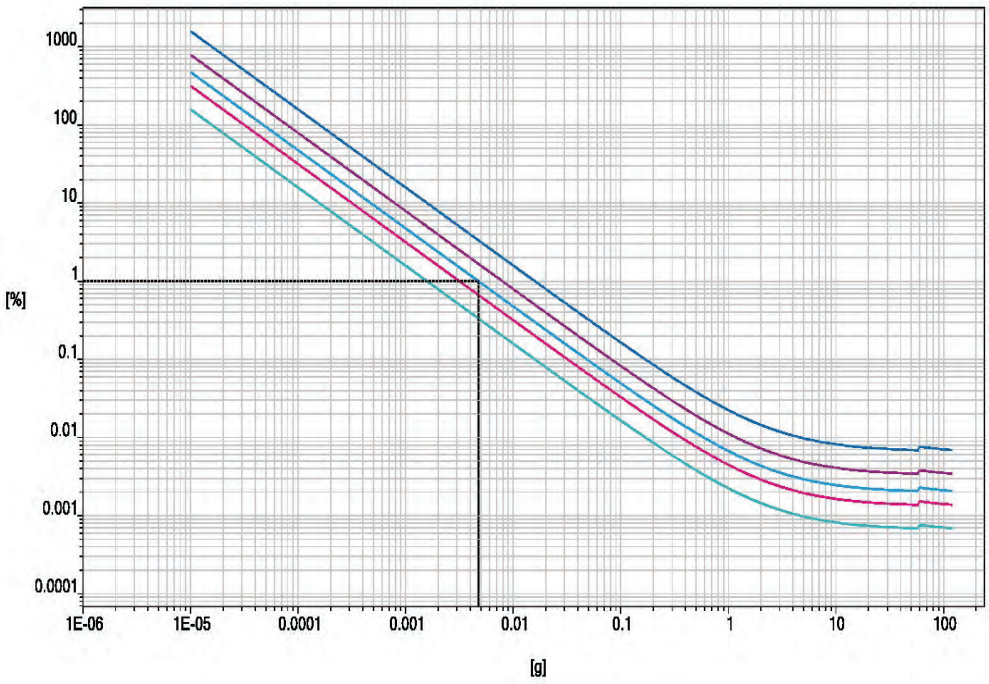

Safety factor
10
5
3
2
1

Displayed example

Process accuracy	1.00 %
Safety factor	3
Minimum sample weight	0.00474 g

© 2024 by Agilent Technologies

Agilent CrossLab Compliance Services

Certificate of System Qualification

GC-OQ + GCMS-OQ

REVIEW BY C. Vue

APPROVED BY Tanyatoom.

NEXT CAL. DATE 25/4/2026

System ID:	GM-3
Organization Name:	ALS Laboratory Group
Organization Location:	104 Phattanakan40, Suan Luang Bangkok 10250
Date:	October 25, 2024 12:05:35 PM
EQP Name:	AgilentRecommended , AgilentRecommended
EQP Revision:	GC.02.52, GCMS.02.53
Overall Qualification Status:	Pass

CDS Logon Verification - GC

Logon: asbkk.env03

Overall CDS Logon Verification - GC Test Status

Pass

System Inspection and Basic Safety and Operation

Name: 7890

Setpoint Status: **Pass**

Overall System Inspection and Basic Safety and Operation Test Status

Pass

Inlet Pressure Accuracy

Name: 7890

Front SSL

Setpoint Status: **Pass**

	Setpoint		Actual	
Inlet Pressure:	25.0	psi	24.9	psi
Accuracy:			0.1	psi
Agilent Recommended:			<= 1.2	

Overall Inlet Pressure Accuracy Test Status

Pass

GC Oven Temperature Accuracy

Name:	7890					
Setpoint Status:	**Pass**					
Zone:	Oven					
	Setpoint/Actual					
Temperature:	230.0	230.9	°C			
Accuracy:		0.9	°C			
Agilent Recommended:	>=	-1.0	% setpoint in K	(	-5.0	°C)
	<=	1.0	% setpoint in K	(	5.0	°C)
Setpoint Status:	**Pass**					
Zone:	Oven					
	Setpoint/Actual					
Temperature:	100.0	100.4	°C			
Accuracy:		0.4	°C			
Agilent Recommended:	>=	-1.0	% setpoint in K	(	-3.7	°C)
	<=	1.0	% setpoint in K	(	3.7	°C)

Overall GC Oven Temperature Accuracy Test Status

Pass

GC Oven Temperature Stability

Name:	7890			
Setpoint Status:	**Pass**			
	Setpoint/Average			
Temperature:	100.0	100.3333	°C	
Stability:		0.1	°C	
Agilent Recommended:	<=	0.5		

Overall GC Oven Temperature Stability Test Status

Pass

Date: October 25, 2024 12:05:35 PM
System ID: GM-3

© 2024 by Agilent Technologies

Log Amp

Tested Combination1 Front SSL / External SQ

Name: 5975C inert XL with TAD

Setpoint Status: **Pass**

Overall Log Amp Test Status

Pass

RFPA

Tested Combination1 Front SSL / External SQ

Name: 5975C inert XL with TAD

Setpoint Status: **Pass**

Amu: 1050 m/z

Drift After Five Minutes: 11 mV

Agilent Recommended: >= -100 and <= 100

RFPA Voltage: 524 mV

Agilent Recommended: <= 1100

Overall RFPA Test Status

Pass

Tune EI

Tested Combination1 Front SSL / External SQ

Name: 5975C inert XL with TAD

Setpoint Status: **Pass**

Filament: 1

Setpoint Status: **Pass**

Filament: 2

Overall Tune EI Test Status

Pass

Scouting Run

Date: October 25, 2024 12:05:35 PM

System ID: GM-3

Tested Combination1 Front SSL / External SQ

Injection Tower

Name: 7693A

Source: EI - Inert

Setpoint Status: **Completed**

Injection Volume on Column: 1.0 uL

Overall Scouting Run Status

Completed

Signal to Noise EI

Tested Combination1 Front **SSL** / External SQ

Name: 5975C inert XL with TAD

Source: EI - Inert Filament: 1

Setpoint Status: **Pass**

Signal to Noise: 1572

Agilent Recommended: >= 320

Source: EI - Inert Filament: 2

Setpoint Status: **Pass**

Signal to Noise: 1541

Agilent Recommended: >= 320

Overall Signal to Noise EI Test Status

Pass

Injection Precision

Tested Combination1 Front **SSL** / External SQ

Name: 7693A

Source: EI - Inert

Date: October 25, 2024 12:05:35 PM

System ID: GM-3

© 2024 by Agilent Technologies

Setpoint Status:	**Pass**				
Injection Volume on Column:	1.0	uL			
Area RSD:	0.61	%	Retention Time RSD:	0.01	%
Agilent Recommended:	<= 5.00			<= 1.00	

Overall Injection Precision Test Status

Pass

Mass Ratio Precision

Tested Combination1 Front SSL / External SQ

Injection Tower

Name: 7693A

Source: EI - Inert

Setpoint Status: **Pass**

Injection Volume on Column: 1.0 uL

	Area Mass 1 Abundance*s		Mass Ratio	
RSD:	0.61	%	0.33	%
Agilent Recommended:	<= 5.00		<= 5.00	
	Pass		Pass	

Overall Mass Ratio Precision Test Status

Pass

Instrument Details

Purpose

This section describes the as found system configuration.

Details

System

System ID	GM-3
Manufacturer	Agilent Technologies
Name	7890
Flow Data Input	Manual Data
Temperature Data Input	Manual Data or Other Data Logging

Tested Combination1

Injection Technique	Injection Tower
Inlet	Front
Detector	External
LTM Included?	No

Sampler 1

Manufacturer	Agilent Technologies
Type	Injection Tower
Name	7693A
Model Number	G4513A
Serial Number	CN12520102
Firmware Revision	A.10.07
Usage	Sample Injection
Location	Front
Syringe Volume (µL)	10

Mainframe 1

Manufacturer	Agilent Technologies
Name	7890
Model Number	G3440A
Serial Number	CN12521119
Firmware Revision	A.01.14
Oven Type	Standard

Inlet 1

Manufacturer	Agilent Technologies
Name	7890
Type	SSL
Location	Front
Carrier Gas	Helium
Control Type	Electronic Pressure Control (EPC)
Purged Inlet	Yes

Detector 1

Manufacturer	Agilent Technologies
Name	Mass Spectrometer
Type	Mass Spectrometer
Location	External

Mass Spectrometer 1

Manufacturer	Agilent Technologies
Type	SQ
Name	5975C inert XL with TAD
Model Number	G3172A
Serial Number	US13013A11
Firmware Revision	7.02.29
High Vacuum System	Turbo Pump
Scouting Run Standard	MRP Std

MS EI Source 1

Manufacturer	Agilent Technologies
Source Type	EI - Inert
Number of filaments	2

Electronic Signature

Purpose

This signature page was created and published because the ACE sign-off action was executed, which is valid for the entire document, including attachments. The ACE sign-off is an electronic signature that requires two distinct identification components: unique username and personal password. The Agilent representative who has delivered this service understands the meaning and legal status of an electronic signature. As a trained official operator, the Agilent representative has a unique password and logon to access ACE and electronically sign this document. (Other e-signatures can be applied to this document using a Document Content Management or other suitable method defined in your data access and control procedures.)

Details

Full Name of Signer:	Adirek Rattanawijit
Logged On User Name:	adirek.rattanawijit@non.agilent.com
Signature Creation Date:	October 25, 2024
Reason for Signature:	Executed protocol and published this original version of document

Regulatory Disclaimer

This document provides a protocol to verify and record instrument configuration and evidence of proper operation. It has been prepared from our interpretation of applicable regulations as well as industry best practices. The document is designed to provide an important component of a complete compliance package. Validation depends upon many factors and use of this protocol alone does not assure compliance. Agilent Technologies makes no promises or representations as to its sufficiency for any specific regulatory program.

Warranty

Agilent Technologies makes no warranty of any kind to this material, including but not limited to, the implied warranties or merchantability and fitness for a particular purpose. Agilent Technologies shall not be liable for errors contained herein or for incidental or consequential damages in connection with the furnishing, performance, or use of this material.

User Name: adirek.rattanawijit System Id: GM-3
Report Generated by Hostname: ASBKKWX314 Print Date: October 25, 2024 12:05:37 PM

ALS_OQGCMS_GM-3_2024 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
October 25, 2024 10:33:46 AM	Audit	SessionCreated	Session	None
October 25, 2024 10:33:46 AM	Start	Configuration	Session	None
October 25, 2024 10:33:46 AM	Audit	Entitlement	Licensing	User is Nonpaying and does not require an unlock code
October 25, 2024 10:41:54 AM	Audit	EqpLoaded	Session	EQP details for primary technique [Gc] - File path: [ProtocolPacks/Gc/Configurations/02.52/Gc.02.52.eqp], EQP File Name: [Gc.02.52.eqp], EQP Name: [AgilentRecommended],Protocol Revision :[Gc.02.52] EQP details for hyphenated technique [GcMs] - File path: [ProtocolPacks/GcMs/Configuretions/02.53/GcMs.02.53.eqp], EQP File Name: [GcMs.02.53.eqp], EQP Name: [AgilentRecommended]
October 25, 2024 10:42:30 AM	End	Configuration	Session	None
October 25, 2024 10:42:32 AM	Start	Qualification	Session	OQ
October 25, 2024 10:42:32 AM	Start	Execution	CDS Logon Verification - GC : - Qualitative test	None
October 25, 2024 10:45:20 AM	End	Execution	CDS Logon Verification - GC : - Qualitative test	Run Count : 1

Page 1 / 11

User Name: adirek.rattanawijit System Id: GM-3
Report Generated by Hostname: ASBKKWX314 Print Date: October 25, 2024 12:05:37 PM

ALS_OQGCMS_GM-3_2024 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
October 25, 2024 10:45:22 AM	Start	Execution	System Inspection and Basic Safety and Operation - 7890: - Qualitative Test - No setpoints associated	None
October 25, 2024 10:45:32 AM	End	Execution	System Inspection and Basic Safety and Operation - 7890: - Qualitative Test - No setpoints associated	Run Count : 1
October 25, 2024 10:45:34 AM	Start	Execution	Inlet Pressure Accuracy - Front SSL: - Pressure Controlled Inlet - S: 25.0 psi - L: <= 1.2 psi	None
October 25, 2024 10:45:38 AM	End	Execution	Inlet Pressure Accuracy - Front SSL: - Pressure Controlled Inlet - S: 25.0 psi - L: <= 1.2 psi	Run Count : 1
October 25, 2024 10:45:40 AM	Start	Execution	GC Oven Temperature Accuracy - 7890: - Temperature : Oven - S: 230.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	None
October 25, 2024 10:46:50 AM	Audit	Data	GC Oven Temperature Accuracy - 7890: - Temperature : Oven - S: 230.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	Manual Data Entry
October 25, 2024 10:46:52 AM	End	Execution	GC Oven Temperature Accuracy - 7890: - Temperature : Oven - S: 230.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	Run Count : 1
October 25, 2024 10:46:54 AM	Start	Execution	GC Oven Temperature Accuracy - 7890: - Temperature : Oven - S: 100.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	None
October 25, 2024 10:47:21 AM	Audit	Data	GC Oven Temperature Accuracy - 7890: - Temperature : Oven - S: 100.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	Manual Data Entry

User Name: adirek.rattanawijit System Id: GM-3
Report Generated by Hostname: ASBKKWX314 Print Date: October 25, 2024 12:05:37 PM

ALS_OQGCMS_GM-3_2024 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
October 25, 2024 10:47:22 AM	End	Execution	GC Oven Temperature Accuracy - 7890: - Temperature : Oven - S: 100.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	Run Count : 1
October 25, 2024 10:47:23 AM	Start	Execution	GC Oven Temperature Stability - 7890: - Temperature : Oven - S: 100.0°C - L: <= 0.5°C	None
October 25, 2024 10:48:14 AM	Audit	Data	GC Oven Temperature Stability - 7890: - Temperature : Oven - S: 100.0°C - L: <= 0.5°C	Manual Data Entry
October 25, 2024 10:48:15 AM	End	Execution	GC Oven Temperature Stability - 7890: - Temperature : Oven - S: 100.0°C - L: <= 0.5°C	Run Count : 1
October 25, 2024 10:48:20 AM	Start	Execution	Log Amp - 5975C inert XL with TAD SQ: - Source: EI - Inert	None
October 25, 2024 10:52:15 AM	End	Execution	Log Amp - 5975C inert XL with TAD SQ: - Source: EI - Inert	Run Count : 1
October 25, 2024 10:52:18 AM	Start	Execution	RFPA - 5975C inert XL with TAD SQ: - Source: EI - Inert	None
October 25, 2024 10:55:41 AM	Start	Execution	Tune EI - 5975C inert XL with TAD SQ: - Source: - EI - Inert Filament 1 (Qualitative - No setpoints associated)	None
October 25, 2024 10:56:55 AM	End	Execution	Tune EI - 5975C inert XL with TAD SQ: - Source: - EI - Inert Filament 1 (Qualitative - No setpoints associated)	Run Count : 1
October 25, 2024 10:56:58 AM	Start	Execution	Tune EI - 5975C inert XL with TAD SQ: - Source: - EI - Inert Filament 2 (Qualitative - No setpoints associated)	None

User Name: adirek.rattanawijit System Id: GM-3
Report Generated by Hostname: ASBKKWX314 Print Date: October 25, 2024 12:05:37 PM

ALS_OQGCMS_GM-3_2024 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
October 25, 2024 10:57:25 AM	End	Execution	Tune EI - 5975C inert XL with TAD SQ: - Source: - EI - Inert Filament 2 (Qualitative - No setpoints associated)	Run Count : 1
October 25, 2024 10:57:32 AM	Start	Execution	Scouting Run - Injection Tower, Front SSL, SQ: - Source: - EI - Inert- Part of GCMS System Preparation	None
October 25, 2024 10:59:48 AM	Audit	Data	Scouting Run - Injection Tower, Front SSL, SQ: - Source: - EI - Inert- Part of GCMS System Preparation	Data files Path : D:\MassHunter\GCMS\1\data \OQPV2024\Scout_001.D
October 25, 2024 11:00:27 AM	Audit	Reporting	Reintegration	Reintegration Count: 1 -- [Integration Type: injections; BaselineCorrectionMode: Advanced; InitialSlopeSensitivity: 10; InitialPeakWidth: 0.01; InitialAreaReject: 0; InitialHeightReject: 50000; Integration: Off at 0; Integration: On at 5.2;]
October 25, 2024 11:00:31 AM	End	Execution	Scouting Run - Injection Tower, Front SSL, SQ: - Source: - EI - Inert- Part of GCMS System Preparation	Run Count : 1
October 25, 2024 11:00:39 AM	Start	Execution	Signal to Noise EI - Injection Tower, Front SSL, SQ: - Source: EI - Inert using Filament 1 - L: >= 320	None
October 25, 2024 11:01:11 AM	Start	Execution	RFPA - 5975C inert XL with TAD SQ: - Source: EI - Inert	None
October 25, 2024 11:01:37 AM	End	Execution	RFPA - 5975C inert XL with TAD SQ: - Source: EI - Inert	Run Count : 1

Page 4 / 11

User Name: adirek.rattanawijit
Report Generated by Hostname: ASBKKWX314

System Id: GM-3
Print Date: October 25, 2024 12:05:37 PM

ALS_OQGCMS_GM-3_2024 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
October 25, 2024 11:01:51 AM	Start	Execution	Signal to Noise EI - Injection Tower, Front SSL, SQ: - Source: EI - Inert using Filament 1 - L: >= 320	None
October 25, 2024 11:02:02 AM	Audit	Data	Signal to Noise EI - Injection Tower, Front SSL, SQ: - Source: EI - Inert using Filament 1 - L: >= 320	Data files Path : D:\MassHunter\GCMS\1\data \OQPV2024\SN_F1_001.D
October 25, 2024 11:04:30 AM	Audit	Reporting	Reintegration	Reintegration Count: 1 -- [Integration Type: injections; BaselineCorrectionMode: Advanced; InitialSlopeSensitivity: 10; InitialPeakWidth: 0.01; InitialAreaReject: 0; InitialHeightReject: 1000; Integration: Off at 0; Integration: On at 4; Integration: Off at 5.6;]
October 25, 2024 11:04:41 AM	Audit	Reporting	Reintegration	Reintegration Count: 2 -- [Integration Type: injections; BaselineCorrectionMode: Advanced; InitialSlopeSensitivity: 10; InitialPeakWidth: 0.01; InitialAreaReject: 0; InitialHeightReject: 2000; Integration: Off at 0; Integration: On at 4; Integration: Off at 5.6;]

User Name: adirek.rattanawijit System Id: GM-3
Report Generated by Hostname: ASBKKWX314 Print Date: October 25, 2024 12:05:37 PM

ALS_OQGCMS_GM-3_2024 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
October 25, 2024 11:04:50 AM	Audit	Reporting	Reintegration	Reintegration Count: 3 -- [Integration Type: injections; BaselineCorrectionMode: Advanced; InitialSlopeSensitivity: 10; InitialPeakWidth: 0.01; InitialAreaReject: 0; InitialHeightReject: 2200; Integration: Off at 0; Integration: On at 4; Integration: Off at 5.6;]
October 25, 2024 11:05:02 AM	Audit	Reporting	Reintegration	Reintegration Count: 4 -- [Integration Type: injections; BaselineCorrectionMode: Advanced; InitialSlopeSensitivity: 10; InitialPeakWidth: 0.01; InitialAreaReject: 0; InitialHeightReject: 3000; Integration: Off at 0; Integration: On at 4; Integration: Off at 5.6;]
October 25, 2024 11:05:09 AM	Audit	Reporting	Reintegration	Reintegration Count: 5 -- [Integration Type: injections; BaselineCorrectionMode: Advanced; InitialSlopeSensitivity: 10; InitialPeakWidth: 0.01; InitialAreaReject: 0; InitialHeightReject: 4000; Integration: Off at 0; Integration: On at 4; Integration: Off at 5.6;]
October 25, 2024 11:16:07 AM	Start	Execution	Signal to Noise EI - Injection Tower, Front SSL, SQ: - Source: EI - Inert using Filament 1 - L: >= 320	None

User Name: adirek.rattanawijit
Report Generated by Hostname: ASBKKWX314

System Id: GM-3
Print Date: October 25, 2024 12:05:37 PM

ALS_OQGCMS_GM-3_2024 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
October 25, 2024 11:28:50 AM	Start	Execution	Signal to Noise EI - Injection Tower, Front SSL, SQ: - Source: EI - Inert using Filament 1 - L: >= 320	None
October 25, 2024 11:29:20 AM	End	Execution	Signal to Noise EI - Injection Tower, Front SSL, SQ: - Source: EI - Inert using Filament 1 - L: >= 320	Run Count : 1
October 25, 2024 11:29:23 AM	Start	Execution	Injection Precision - Injection Tower, Front SSL, SQ: - Source: - EI - Inert L (Area): <= 5.00% - L (Ret. Time): <= 1.00%	None
October 25, 2024 11:29:36 AM	Audit	Data	Injection Precision - Injection Tower, Front SSL, SQ: - Source: - EI - Inert L (Area): <= 5.00% - L (Ret. Time): <= 1.00%	Data files Path : D:\MassHunter\GCMS\1\data \OQPV2024\MRP_002.D
October 25, 2024 11:29:36 AM	Audit	Data	Injection Precision - Injection Tower, Front SSL, SQ: - Source: - EI - Inert L (Area): <= 5.00% - L (Ret. Time): <= 1.00%	Data files Path : D:\MassHunter\GCMS\1\data \OQPV2024\MRP_003.D
October 25, 2024 11:29:36 AM	Audit	Data	Injection Precision - Injection Tower, Front SSL, SQ: - Source: - EI - Inert L (Area): <= 5.00% - L (Ret. Time): <= 1.00%	Data files Path : D:\MassHunter\GCMS\1\data \OQPV2024\MRP_004.D
October 25, 2024 11:29:36 AM	Audit	Data	Injection Precision - Injection Tower, Front SSL, SQ: - Source: - EI - Inert L (Area): <= 5.00% - L (Ret. Time): <= 1.00%	Data files Path : D:\MassHunter\GCMS\1\data \OQPV2024\MRP_005.D
October 25, 2024 11:29:37 AM	Audit	Data	Injection Precision - Injection Tower, Front SSL, SQ: - Source: - EI - Inert L (Area): <= 5.00% - L (Ret. Time): <= 1.00%	Data files Path : D:\MassHunter\GCMS\1\data \OQPV2024\MRP_006.D

User Name: adirek.rattanawijit
Report Generated by Hostname: ASBKKWX314

System Id: GM-3
Print Date: October 25, 2024 12:05:37 PM

ALS_OQGCMS_GM-3_2024 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
October 25, 2024 11:29:37 AM	Audit	Data	Injection Precision - Injection Tower, Front SSL, SQ: - Source: - EI - Inert L (Area): <= 5.00% - L (Ret. Time): <= 1.00%	Data files Path : D:\MassHunter\GCMS\1\data \OQPV2024\MRP_007.D
October 25, 2024 11:29:47 AM	Audit	Reporting	Reintegration	Reintegration Count: 1 -- [Integration Type: injections; BaselineCorrectionMode: Advanced; InitialSlopeSensitivity: 10; InitialPeakWidth: 0.01; InitialAreaReject: 0; InitialHeightReject: 50000; Integration: Off at 0; Integration: On at 5.2;]
October 25, 2024 11:29:48 AM	End	Execution	Injection Precision - Injection Tower, Front SSL, SQ: - Source: - EI - Inert L (Area): <= 5.00% - L (Ret. Time): <= 1.00%	Run Count : 1
October 25, 2024 11:29:51 AM	Start	Execution	Mass Ratio Precision - Injection Tower, Front SSL, SQ: - Source: EI - Inert - L (RSD): <= 5.00%	None
October 25, 2024 11:30:04 AM	Audit	Data	Mass Ratio Precision - Injection Tower, Front SSL, SQ: - Source: EI - Inert - L (RSD): <= 5.00%	Data files Path : D:\MassHunter\GCMS\1\data \OQPV2024\MRP_002.D
October 25, 2024 11:30:04 AM	Audit	Data	Mass Ratio Precision - Injection Tower, Front SSL, SQ: - Source: EI - Inert - L (RSD): <= 5.00%	Data files Path : D:\MassHunter\GCMS\1\data \OQPV2024\MRP_003.D
October 25, 2024 11:30:04 AM	Audit	Data	Mass Ratio Precision - Injection Tower, Front SSL, SQ: - Source: EI - Inert - L (RSD): <= 5.00%	Data files Path : D:\MassHunter\GCMS\1\data \OQPV2024\MRP_004.D

User Name: adirek.rattanawijit
Report Generated by Hostname: ASBKKWX314

System Id: GM-3
Print Date: October 25, 2024 12:05:37 PM

ALS_OQGCMS_GM-3_2024 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
October 25, 2024 11:30:04 AM	Audit	Data	Mass Ratio Precision - Injection Tower, Front SSL, SQ: - Source: EI - Inert - L (RSD): <= 5.00%	Data files Path : D:\MassHunter\GCMS\1\data \OQPV2024\MRP_005.D
October 25, 2024 11:30:04 AM	Audit	Data	Mass Ratio Precision - Injection Tower, Front SSL, SQ: - Source: EI - Inert - L (RSD): <= 5.00%	Data files Path : D:\MassHunter\GCMS\1\data \OQPV2024\MRP_006.D
October 25, 2024 11:30:04 AM	Audit	Data	Mass Ratio Precision - Injection Tower, Front SSL, SQ: - Source: EI - Inert - L (RSD): <= 5.00%	Data files Path : D:\MassHunter\GCMS\1\data \OQPV2024\MRP_007.D
October 25, 2024 11:30:15 AM	Audit	Reporting	Reintegration	Reintegration Count: 1 -- [Integration Type: injections; BaselineCorrectionMode: Advanced; InitialSlopeSensitivity: 10; InitialPeakWidth: 0.01; InitialAreaReject: 0; InitialHeightReject: 50000; Integration: Off at 0; Integration: On at 5.2;]
October 25, 2024 11:30:17 AM	End	Execution	Mass Ratio Precision - Injection Tower, Front SSL, SQ: - Source: EI - Inert - L (RSD): <= 5.00%	Run Count : 1
October 25, 2024 11:30:23 AM	End	Qualification	Session	OO
October 25, 2024 11:30:23 AM	Start	Reporting	Session	None
October 25, 2024 11:34:59 AM	End	Reporting	Session	None
October 25, 2024 11:34:59 AM	Start	Qualification	Session	OQ

User Name: adirek.rattanawijit
Report Generated by Hostname: ASBKKWX314

System Id: GM-3
Print Date: October 25, 2024 12:05:37 PM

ALS_OQGCMS_GM-3_2024 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
October 25, 2024 11:44:32 AM	Start	Execution	Signal to Noise EI - Injection Tower, Front SSL, SQ: - Source: EI - Inert using Filament 2 - L: >= 320	None
October 25, 2024 11:44:39 AM	Audit	Data	DataManager	DataManager was in a data verification state but the user chose to start over
October 25, 2024 11:44:42 AM	Audit	Data	Signal to Noise EI - Injection Tower, Front SSL, SQ: - Source: EI - Inert using Filament 2 - L: >= 320	Data files Path : D:\MassHunter\GCMS\1\data \OQPV2024\SN_F2_001.D
October 25, 2024 11:44:53 AM	Audit	Reporting	Reintegration	Reintegration Count: 1 -- [Integration Type: injections; BaselineCorrectionMode: Advanced; InitialSlopeSensitivity: 10; InitialPeakWidth: 0.01; InitialAreaReject: 0; InitialHeightReject: 1000; Integration: Off at 0; Integration: On at 4;]
October 25, 2024 11:45:20 AM	Audit	Reporting	Reintegration	Reintegration Count: 2 -- [Integration Type: injections; BaselineCorrectionMode: Advanced; InitialSlopeSensitivity: 10; InitialPeakWidth: 0.01; InitialAreaReject: 0; InitialHeightReject: 1000; Integration: Off at 0; Integration: On at 5; Integration: Off at 7;]
October 25, 2024 11:45:34 AM	End	Execution	Signal to Noise EI - Injection Tower, Front SSL, SQ: - Source: EI - Inert using Filament 2 - L: >= 320	Run Count : 1

User Name: adirek.rattanawijit System Id: GM-3
Report Generated by Hostname: ASBKKWX314 Print Date: October 25, 2024 12:05:37 PM

ALS_OQGCMS_GM-3_2024 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
October 25, 2024 11:45:59 AM	End	Qualification	Session	OQ
October 25, 2024 11:45:59 AM	Start	Reporting	Session	None
October 25, 2024 12:03:37 PM	Audit	Reporting	Session	Report Generated : Certificate
October 25, 2024 12:04:58 PM	Audit	Reporting	Session	Report Generated : Report

JIRANATEE ASSOCIATES CO.,LTD.

TEST REPORT

CUSTOMER NAME	: ALS Laboratory Group (Thailand) Co., Ltd. [บริษัท เอแอลเอส แลบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด]				
EQRIPMENT NAME	: THC Analyzer				
MANUFACTURER	: HORIBA	MODEL	: APHA-370	SERIAL NO	: U430GTHB
STANDARD GAS CONCENTRATION (PPM) (CH4) :	506.1 PPM			CYLINDER NO	: CC734373
CYLINDER PRESSURE (pslg) :	1,600 PSI			CERTIFIED DATE	: 12/05/2020
CERTIFIED BY :	AIRGAS			EXPIRED DATE	: 12/05/2028

TEST RESULTS

POINT NO	TEST RESULTS						
	IDEAL	ACTUAL CH4	ERROR CH4	%ERROR CH4	ACTUAL THC	ERROR THC	%ERROR THC
ZERO	0.00	0.00	0.00	-	0.00	0.00	-
1	10.00	10.05	0.05	0.50	10.05	0.05	0.50
2	20.00	20.10	0.10	0.50	20.12	0.12	0.60
3	30.00	30.29	0.29	0.97	30.27	0.27	0.90
4	40.00	40.01	0.01	0.02	40.02	0.02	0.05
AVERAGE (%)				0.50			0.51

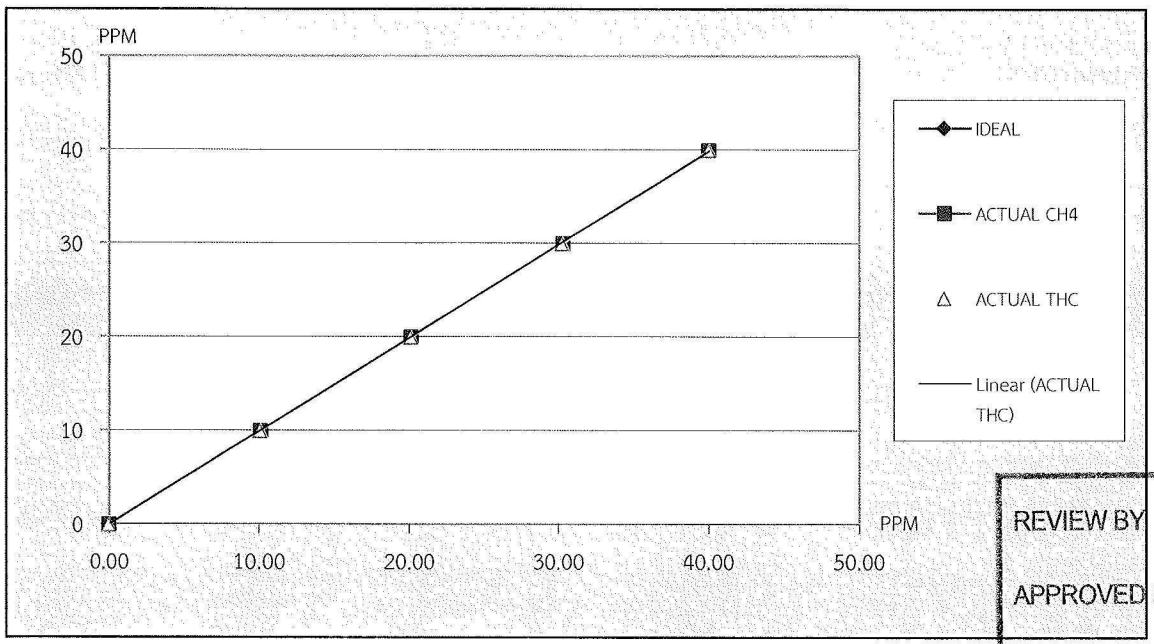

REVIEW BY Thanitsl.

APPROVED BY

NEXT CAL. DATE 6/03/2026

CALIBRATED BY : สุทธิชา คงสอน DATE : 6/3/68

CHECKED BY : สันติ ปัดมะ DATE : 6/3/68

JIRANATEE ASSOCIATES CO.,LTD.

ต้องการข้อมูลทางด้านเทคนิคเพิ่มเติม : เจ้าหน้าที่ฝ่ายบริการหลังการขาย , โทร 02-868-0812 # 15,16 , E-Mail : Engineer@jiranatee.com
เลขที่ 63/14-15,67/35-36 ถนนเพชรเกษม 7,7/1 แขวงวัดท่าพระ เขตบางกอกใหญ่ กรุงเทพฯ 10600 โทร 02-8680812-13 โทรสาร 02-868-1889

JIRANATEE ASSOCIATES CO.,LTD.

CHECK LIST

CUSTOMER NAME	: ALS Laboratory Group (Thailand) Co., Ltd. [บริษัท เอแอลเอส แลบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด]		
EQUIPMENT NAME	: THC Analyzer		
MANUFACTURER	: HORIBA	MODEL : APHA-370	SERIAL NO. : U430GTHB

TEST VALUES

NO.	THC Analyzer (APHA - 370)	UNIT	BEFORE	AFTER
1	Signal (CH4)	mV	35.50	35.40
2	Signal (THC)	mV	38.40	50.10
3	Detector	Temp °C , Standard Value : Ambient temp+(5°Cto15°C)	45.20	45.80
		Pressure kPa , Standard Value : (Ambient/1013x100-20)±4kPa	69.50	69.50
4	Ambient	kPa current atmospheric pressure	100.60	100.50
5	Purlifire	°C , Standard Value : 390 °C to 430 °C	419.90	419.80
		kPa , Normal value : 8 kPa to 25 kPa	9.70	9.70
6	NMHC	°C , Standard Value : 230 °C to 260 °C	244.00	244.10
7	DC 24 V	V , Standard Value : 24 V ± 0.5 V	23.90	23.90
8	DC 5 V	V , Standard Value : 5 V ± 0.5 V	5.00	5.00
9	Bypass (Optional)	L/min, Normal value : 0.9 L/min ± 0.3 L/min	-	-
10	Over Flow (Optional)	L/min, Standard Value : 0.8 L/min or More	-	-
11	CH4 Samping Reading	PPM	2.08	2.07
12	NMHC Samping Reading	PPM	0.06	0.75
13	THC Samping Reading	PPM	2.14	2.82
14	Zero Gas CH4/THC	PPM	0.02/-0.02	0.00/0.00
15	Span Gas	PPM	39.66/39.70	40.01/40.02
G	Gas H2 ...../.....	20 PSI	20	20

Remark : Reference EX-EN-017-56 , Ambient HC Monitor APHA-370 Operetion Manual Page #81

Remark : (Ambeint temperature = 5°C to 40°C)

อาการที่ตรวจพบ

- Service Maintenance

รายละเอียดการดำเนินการ

- ทำการ Service Maintenance , ทำ Calibration Zero/Span , Multipoint

ผลการดำเนินการ

- เรียบร้อย เครื่องสามารถดำเนินการตรวจวัดได้ตามปกติ

CALIBRATED BY : ศิริชัย ฉลอง DATE : 6/3/68

CHECKED BY : ชัยณรงค์ ปัญญะ DATE : 6/3/68

JIRANATEE ASSOCIATES CO.,LTD.

ต้องการข้อมูลทางด้านเทคนิคเพิ่มเติม : เจ้าหน้าที่ฝ่ายบริการหลังการขาย , โทร 02-868-0812 # 15-16 , E-Mail : Engineer@jiranatee.com

เลขที่ 63/14-15,67/35-36 ซอยเพชรเกษม 7,7/1 ถนนเพชรเกษม แขวงวัดท่าพระ เขตบางกอกใหญ่ กรุงเทพฯ 10600 โทร 02-868-0812-13 โทรสาร 02-868-1889

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7/139 MOO 13, SOI SUNTINAKORN 11 TAMBON BANG KAEO,
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL: (66)0-2116-5860-1 FAX: (66)0-2116-7140

Certificate of Calibration

Customer

Name : ALS Laboratory Group Thailand Co., Ltd.

Address : 104 Soi Phatthanakan 40, Phatthanakan Road, Suan Luang, Bangkok 10250

Certificate No : 25-ACT-010

Request No : Req-2025-0091

Unit Under Calibration Details

Measurement item : Acoustic Calibrator

Manufacturer : RION

Model : NC-74

Serial Number : 34178121

ID : RYG_FS0213

Class : 1

Range : 94 dB / 1000 Hz

Instrument Status : Used

REVIEW BY .....

APPROVED BY.....

NEXT CAL DATE.....16/01/26

Calibration Environment and Details

Temperature : (23 ±2 ˚C)

Humidity : (50 ± 20 %RH)

Barometric Pressure : (1013 ±10.0 hPa)

Received Date : 15 January 2025

Calibration Date : 16 January 2025

Location of Calibration : LAB 1 Acoustic

Calibration Procedure : In-house method CP-ACT-02 based on IEC 60942:2017 Electroacoustics - Sound calibrators

Reference Standard	Model	Serial Number	Traceable	Due Calibration
Sound Calibrator	SV 35A	58079	EEI	12 June 2025
THD Multimeter	2015	1047765	NIMT	16 January 2025

Traceability : This certificate providoes traceability of measurement to recognized national standard, and to the realization of the international System of Units (SI).

Note

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor k =2, providing a level of confidence approximately 95 %.

Calibrated By :

Mr. Noppadon Luangart

Service Calibration Engineer

Approved By :

Mr. Pacit Mathavorn

Calibration Engineer Supervisor

Issue Date : 16 January 2025

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7/139 MOO 13, SOI SUNTINAKORN 11 TAMBON BANG KAEO,
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL: (66)0-2116-5860-1 FAX: (66)0-2116-7140

Certificate No : 25-ACT-010

Request No : Req-2025-0091

Sound pressure level **Calibration Results :** Without Adjustment

Calibration Range (dB)	Without Adjustment (dB)		Adjustment (dB)		Uncertainty (± dB)	Acceptance limit Class 1 (± dB)	Result
	Measured	Deviated value	Measured	Deviated value			
94 dB / 1000 Hz	94.11	0.11	-	-	0.13	0.25	Pass

Frequency of Sound pressure level

Calibration Range (Hz)	Without Adjustment		Adjustment		Uncertainty (± %)	Acceptance limit Class 1 (± %)	Result
	Measured (Hz)	Deviated	Measured (Hz)	Deviated			
94 dB / 1000 Hz	1000.00	0.00	-	-	0.01	0.70	Pass

Total Harmonic Distortion plus Noise of Sound pressure level (THD+N %)

Calibration Range (Hz)	Without Adjustment	Adjustment	Uncertainty (± %)	Acceptance limit Class 1 (± %)	Result
	Measured (%)	Measured (%)			
94 dB / 1000 Hz	1.21	-	0.40	2.5	Pass

Note :

Function	Maximum-permitted Uncertainty of measurement
Sound pressure level	0.15 dB
Frequency	0.20%
Total distortion+noise	0.50%

- Acceptance limit was IEC60942:2017 Class 1

- The calibration results exclude the calibrator pressure correction

- The calibration results exclude the microphone volume correction

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7/139 MOO 13, SOI SUNTINAKORN 11 TAMBON BANG KAEO,
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL: (66)0-2116-5860-1 FAX: (66)0-2116-7140

Certificate No : 25-ACT-010

Request No : Req-2025-0091

Decision Rule for Statements of Conformity

The standard decision rule employed for the statements of conformity to each calibration result will be applied using ILAC-G8:09/2019; Guidelines on the Reporting of Compliance with Specification as following Fig. and statements

Pass = The measurement result plus the expanded uncertainty with a 95% coverage probability were within the limit.

Pass[1] = The measurement result was within the limit. However, a portion of the expanded uncertainty of measurement at 95% exceeds the limit.

Fail[1] = The measurement result was out of the limit. However, a portion of the expanded uncertainty of measurement at 95% is within the limit.

Fail = The measurement result plus the expanded uncertainty with a 95% coverage probability were outside the limit.

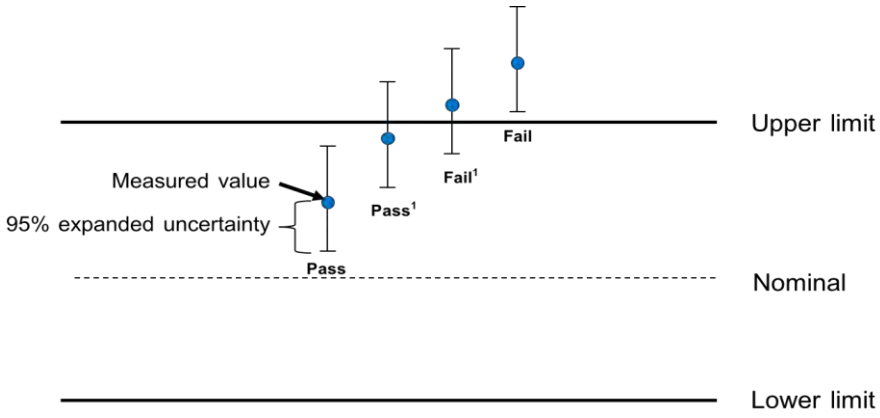

End of Calibration

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

SITHIPORN ASSOCIATES CO., LTD.
CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand
Tel. +66 2433 8331 Email : calibration@sithiphorn.com

NSC-TISI-TIS 17025
CALIBRATION 0394

Calibration Certificate

Equipment :	SOUND LEVEL METER
Manufacturer :	RION
Model :	NL-42 / Microphone UC-52 / Preamplifier NH-24
Serial No.:	00873057 / 171591 / 73333
ID No.:	RYG_FS0381

Condition As Found : GOOD

Customer : ALS LABORATORY GROUP (THAILAND) CO., LTD.
104 PHATTHANAKAN 40, PHATTHANAKAN ROAD,
KHWAENG PHATTHANAKAN, KHET SUAN LUANG,
BANGKOK, 10250 THAILAND.

Location :	-	
Ambient Temperature :	(23.0 ± 3)	°C
Pressure :	(101.3 ± 3)	kPa
Relative Humidity :	(50.0 ± 20)	%

REVIEW BY Wanakorn P.
APPROVED BY
NEXT CAL. DATE 9/10/25

Received Date :	23 SEPTEMBER 2024
Calibration Date :	09 OCTOBER 2024
Date of Issue :	09 OCTOBER 2024

Calibrated by : Nathakorn Pisutpaisan

Approved by :
(Thanakul Petchurai)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

SITHIPORN ASSOCIATES CO., LTD.
CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand
Tel. +66 2433 8331 Email : calibration@sithiphorn.com

SITHIPORN associates

NSC-TISI-TIS 17025
CALIBRATION 0394

Calibration Procedure : CP-AC-01

Calibration Method :

This equipment was calibrated by follow on IEC-61672-3 (2013) Standard for sound level meter (SLM).

The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.

For tests results of each items were made by observation of each Instruments display and also with SLM's display.

Condition of this result of calibration :

1. Reference Standard Instruments :

Instrument	Model	Serial No.	Cert. No.	Due Date
Waveform Generator	33210A	MY48017076	EF-0009-24	05-FEB-25
Waveform Generator	33511B	MY52302742	EF-0007-24	05-FEB-25
Digital Multimeter	33461A	MY53220104	EEL.BP 21/0267	13-FEB-25
Digital Multimeter	33461A	MY53220076	EEL.BP 20/0267	15-FEB-25
Digital Multimeter	34461A	MY60024273	EEL.BP 22/0267	15-FEB-25
Programmable Attenuator	MAT-1070	62100114	EF-0008-24	05-FEB-25
Condenser Microphone	4180	2977900	AA-1001-24	12-FEB-25
Measuring Amplifier	NA-42KAI	34560495	AA-3001-24	05-FEB-25

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.
3. This certificate is traceable to the international system of unit maintained at :
   - 3.1 National Institute of Metrology (Thailand).
   - 3.2 Thailand Institute of Scientific and Technological Research (TISTR).

SITHIPORN ASSOCIATES CO., LTD.
CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand
Tel. +66 2433 8331 Email : calibration@sithiphorn.com

SITHIPORN associates

NSC-TISI-TIS 17025
CALIBRATION 0394

Cert. No. : ACL24304
Job No. : VC67AC0164
Pages : 3 of 8

Summary of Measurement Result :

Parameter	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	0.2	N/A
2. Self-generated noise	0.2	N/A
3. Acoustical signal tests of frequency weightings		
125 Hz	0.3	0.6
1000 Hz	0.3	0.6
8000 Hz	0.3	0.7
4. Electrical signal tests of frequency weightings		
For 10 Hz to 4 kHz	0.3	0.6
For > 4 kHz to 10 kHz	0.3	0.7
For > 10 kHz to 20 kHz	0.3	1.0
5. Frequency and time weightings at 1 kHz	0.2	0.2
6. Long - term stability	0.1	0.1
7. Level linearity on the reference level range	0.2	0.3
8. Level linearity including the level range control	0.2	0.3
9. Tone burst response	0.2	0.3
10. Peak C sound level	0.2	0.35
11. Overload indication	0.2	0.25
12. High level stability	0.1	0.1

SITHIPORN ASSOCIATES CO., LTD.
CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand
Tel. +66 2433 8331 Email : calibration@sithiphorn.com

SITHIPORN associates

NSC-TISI-TIS 17025
CALIBRATION 0394

Result of calibration :

1. Absolute sensitivity

Reference Acoustic Signal (dB)	Measured Value (dB)	Deviation (dB)	Acceptance Limit (dB)
93.9 (93.94)	93.9	0.0	±0.3

2. Self-generated noise

2.1 Normal test

Measured Value (dB)
16.7

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Weighting (dB)
A - weight	13.4
C - weight	19.3
Flat	25.0

3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
125	0.3	0.4	0.4	± 1.5
1000	0.1	0.1	0.1	± 1.0
8000	1.1	1.2	1.2	±5.0

SITHIPORN ASSOCIATES CO., LTD.
CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand
Tel. +66 2433 8331 Email : calibration@sithiphorn.com

SITHIPORN associates

NSC-TISI-TIS 17025
CALIBRATION 0394

4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	0.0	0.0	0.0	±2.0
125	0.1	0.1	0.1	±1.5
250	0.1	0.0	0.0	±1.5
500	0.0	0.1	0.0	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.1	0.0	±2.0
4000	0.0	0.0	0.0	±3.0
8000	0.0	0.1	0.1	±5.0

5. Frequency and time weightings at 1 kHz

5.1 Frequency weightings at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.2
C - weight	94.0	94.0	0.0	± 0.2
Flat	94.0	94.0	0.0	± 0.2

5.2 Time weighting at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	94.0	94.0	0.0	± 0.1
Slow	94.0	94.0	0.0	± 0.1
Leq	94.0	94.0	0.0	± 0.1

6. Long - term stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.1	0.1	± 0.3

SITHIPORN ASSOCIATES CO., LTD.
CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand
Tel. +66 2433 8331 Email : calibration@sithiphorn.com

SITHIPORN associates

NSC-TISI-TIS 17025
CALIBRATION 0394

7. Level linearity on the reference level range

Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
137.0	137.0	0.0	± 1.1
136.0	136.0	0.0	± 1.1
135.0	135.0	0.0	± 1.1
134.0	134.0	0.0	± 1.1
133.0	133.0	0.0	± 1.1
132.0	132.0	0.0	± 1.1
131.0	131.0	0.0	± 1.1
129.0	129.0	0.0	± 1.1
124.0	124.0	0.0	± 1.1
119.0	119.0	0.0	± 1.1
114.0	114.0	0.0	± 1.1
109.0	109.0	0.0	± 1.1
104.0	104.0	0.0	± 1.1
99.0	99.0	0.0	± 1.1
94.0	94.0	0.0	± 1.1
89.0	89.0	0.0	± 1.1
84.0	84.0	0.0	± 1.1
79.0	79.0	0.0	± 1.1
74.0	74.0	0.0	± 1.1
69.0	69.0	0.0	± 1.1
64.0	64.0	0.0	± 1.1
59.0	59.0	0.0	± 1.1
54.0	54.0	0.0	± 1.1
49.0	49.0	0.0	± 1.1
44.0	44.0	0.0	± 1.1
39.0	39.0	0.0	± 1.1
34.0	34.0	0.0	± 1.1
30.0	30.1	0.1	± 1.1
29.0	29.0	0.0	± 1.1
28.0	28.1	0.1	± 1.1
27.0	27.1	0.1	± 1.1
26.0	26.2	0.2	± 1.1
25.0	25.2	0.2	± 1.1

SITHIPORN ASSOCIATES CO., LTD.
CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand
Tel. +66 2433 8331 Email : calibration@sithiphorn.com

SITHIPORN associates

NSC-TISI-TIS 17025
CALIBRATION 0394

8. Level linearity including the level range control

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
130	94.0	94.0	0.0	±1.1

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
130	30.0	30.1	0.1	±1.1

9. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Cycle	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.1	0.1	±1.0
Slow	2	8	108.0	108.0	0.0	1.5 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
SEL	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.1	0.1	±1.0

SITHIPORN ASSOCIATES CO., LTD.
CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand
Tel. +66 2433 8331 Email : calibration@sithiphorn.com

SITHIPORN associates

NSC-TISI-TIS 17025
CALIBRATION 0394

10. Peak C sound level

Number of cycle in test signal	Anticipated Value (dB)	Measured Value, Lcpeak (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	±3.0
One	136.4	135.9	-0.5	±3.0

Number of cycle in test signal	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.1	0.1	±2.0
Positive half cycle	135.4	135.2	-0.2	±2.0
Negative half cycle	135.4	135.2	-0.2	±2.0

11. Overload indication

Measured value (dB)		Deviated Value (dB)	Acceptance Limits (dB)
Positive one-half cycle	Negative one-half cycle		
89.6	89.5	-0.1	±1.5

12. High level stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor $k = 2$ or any value following calculation,providing a lavel of confidence of approximately 95 %

End of Calibration Certificate

SITHIPORN ASSOCIATES CO., LTD.
CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand
Tel. +66 2433 8331 Email : calibration@sithiphorn.com

NSC-TISI-TIS 17025
CALIBRATION 0394

Cert. No. : ACL24305

Calibration Certificate

Equipment :	SOUND LEVEL METER
Manufacturer :	RION
Model :	NL-42 / Microphone UC-52 / Preamplifier NH-24
Serial No.:	00873109 / 171842 / 73485
ID No.:	RYG_FS0384

Condition As Found : GOOD

Customer : ALS LABORATORY GROUP (THAILAND) CO., LTD.
104 PHATTHANAKAN 40, PHATTHANAKAN ROAD,
KHWAENG PHATTHANAKAN, KHET SUAN LUANG,
BANGKOK, 10250 THAILAND.

Location :	-	
Ambient Temperature :	(23.0 ± 3)	°C
Pressure :	(101.3 ± 3)	kPa
Relative Humidity :	(50.0 ± 20)	%

REVIEW BY Narakorn P.
APPROVED BY
NEXT CAL. DATE 9/10/25

Received Date :	23 SEPTEMBER 2024
Calibration Date :	09 OCTOBER 2024
Date of Issue :	09 OCTOBER 2024

Calibrated by : Nathakorn Pisutpaisan

Approved by :

(Thanakul Petchurai)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

SITHIPORN ASSOCIATES CO., LTD.
CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand
Tel. +66 2433 8331 Email : calibration@sithiphorn.com

NSC-TISI-TIS 17025
CALIBRATION 0394

Calibration Procedure : CP-AC-01

Calibration Method :

This equipment was calibrated by follow on IEC-61672-3 (2013) Standard for sound level meter (SLM).
The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.
For tests results of each items were made by observation of each Instruments display and also with SLM's display.

Condition of this result of calibration :

1. Reference Standard Instruments :

Instrument	Model	Serial No.	Cert. No.	Due Date
Waveform Generator	33210A	MY48017076	EF-0009-24	05-FEB-25
Waveform Generator	33511B	MY52302742	EF-0007-24	05-FEB-25
Digital Multimeter	33461A	MY53220104	EEL.BP 21/0267	13-FEB-25
Digital Multimeter	33461A	MY53220076	EEL.BP 20/0267	15-FEB-25
Digital Multimeter	34461A	MY60024273	EEL.BP 22/0267	15-FEB-25
Programmable Attenuator	MAT-1070	62100114	EF-0008-24	05-FEB-25
Condenser Microphone	4180	2977900	AA-1001-24	12-FEB-25
Measuring Amplifier	NA-42KAI	34560495	AA-3001-24	05-FEB-25

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.
3. This certificate is traceable to the international system of unit maintained at :
   - 3.1 National Institute of Metrology (Thailand).
   - 3.2 Thailand Institute of Scientific and Technological Research (TISTR).

SITHIPORN ASSOCIATES CO., LTD.
CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand
Tel. +66 2433 8331 Email : calibration@sithiphorn.com

SITHIPORN associates

NSC-TISI-TIS 17025
CALIBRATION 0394

Cert. No. : ACL24305
Job No. : VC67AC0164
Pages : 3 of 8

Summary of Measurement Result :

Parameter	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	0.2	N/A
2. Self-generated noise	0.2	N/A
3. Acoustical signal tests of frequency weightings		
125 Hz	0.3	0.6
1000 Hz	0.3	0.6
8000 Hz	0.3	0.7
4. Electrical signal tests of frequency weightings		
For 10 Hz to 4 kHz	0.3	0.6
For > 4 kHz to 10 kHz	0.3	0.7
For > 10 kHz to 20 kHz	0.3	1.0
5. Frequency and time weightings at 1 kHz	0.2	0.2
6. Long - term stability	0.1	0.1
7. Level linearity on the reference level range	0.2	0.3
8. Level linearity including the level range control	0.2	0.3
9. Tone burst response	0.2	0.3
10. Peak C sound level	0.2	0.35
11. Overload indication	0.2	0.25
12. High level stability	0.1	0.1

SITHIPORN ASSOCIATES CO., LTD.
CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand
Tel. +66 2433 8331 Email : calibration@sithiphorn.com

SITHIPORN associates

NSC-TISI-TIS 17025
CALIBRATION 0394

Result of calibration :

1. Absolute sensitivity

Reference Acoustic Signal (dB)	Measured Value (dB)	Deviation (dB)	Acceptance Limit (dB)
93.9 (93.94)	93.9	0.0	±0.3

2. Self-generated noise

2.1 Normal test

Measured Value (dB)
16.1

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Weighting (dB)
A - weight	13.1
C - weight	19.8
Flat	25.1

3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
125	0.4	0.5	0.5	± 1.5
1000	0.0	0.0	0.0	± 1.0
8000	-1.4	-1.3	-1.3	±5.0

SITHIPORN ASSOCIATES CO., LTD.
CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand
Tel. +66 2433 8331 Email : calibration@sithiphorn.com

SITHIPORN associates

NSC-TISI-TIS 17025
CALIBRATION 0394

4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	0.0	0.0	0.0	±2.0
125	0.1	0.1	0.0	±1.5
250	0.0	0.0	0.0	±1.5
500	0.0	0.1	0.0	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.1	0.0	±2.0
4000	0.0	0.0	0.0	±3.0
8000	0.0	0.1	0.1	±5.0

5. Frequency and time weightings at 1 kHz

5.1 Frequency weightings at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.2
C - weight	94.0	94.0	0.0	± 0.2
Flat	94.0	94.0	0.0	± 0.2

5.2 Time weighting at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	94.0	94.0	0.0	± 0.1
Slow	94.0	94.0	0.0	± 0.1
Leq	94.0	94.0	0.0	± 0.1

6. Long - term stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.3

SITHIPORN ASSOCIATES CO., LTD.
CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand
Tel. +66 2433 8331 Email : calibration@sithiphorn.com

SITHIPORN associates

NSC-TISI-TIS 17025
CALIBRATION 0394

7. Level linearity on the reference level range

Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
137.0	137.0	0.0	± 1.1
136.0	136.0	0.0	± 1.1
135.0	135.0	0.0	± 1.1
134.0	134.0	0.0	± 1.1
133.0	133.0	0.0	± 1.1
132.0	132.0	0.0	± 1.1
131.0	131.0	0.0	± 1.1
129.0	129.0	0.0	± 1.1
124.0	124.0	0.0	± 1.1
119.0	119.0	0.0	± 1.1
114.0	114.0	0.0	± 1.1
109.0	109.0	0.0	± 1.1
104.0	104.0	0.0	± 1.1
99.0	99.0	0.0	± 1.1
94.0	94.0	0.0	± 1.1
89.0	89.0	0.0	± 1.1
84.0	84.0	0.0	± 1.1
79.0	79.0	0.0	± 1.1
74.0	74.0	0.0	± 1.1
69.0	69.0	0.0	± 1.1
64.0	64.0	0.0	± 1.1
59.0	59.0	0.0	± 1.1
54.0	54.0	0.0	± 1.1
49.0	49.0	0.0	± 1.1
44.0	44.0	0.0	± 1.1
39.0	39.0	0.0	± 1.1
34.0	34.0	0.0	± 1.1
30.0	30.0	0.0	± 1.1
29.0	29.0	0.0	± 1.1
28.0	28.1	0.1	± 1.1
27.0	27.2	0.2	± 1.1
26.0	26.2	0.2	± 1.1
25.0	25.2	0.2	± 1.1

SITHIPORN ASSOCIATES CO., LTD.
CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand
Tel. +66 2433 8331 Email : calibration@sithiphorn.com

SITHIPORN associates

NSC-TISI-TIS 17025
CALIBRATION 0394

8. Level linearity including the level range control

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
130	94.0	94.0	0.0	±1.1

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
130	30.0	30.1	0.1	±1.1

9. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Cycle	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.1	0.1	±1.0
Slow	2	8	108.0	108.0	0.0	1.5 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
SEL	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.1	0.1	±1.0

SITHIPORN ASSOCIATES CO., LTD.
CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand
Tel. +66 2433 8331 Email : calibration@sithiphorn.com

SITHIPORN associates

NSC-TISI-TIS 17025
CALIBRATION 0394

10. Peak C sound level

Number of cycle in test signal	Anticipated Value (dB)	Measured Value, Lcpeak (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	±3.0
One	136.4	136.2	-0.2	±3.0

Number of cycle in test signal	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	±2.0
Positive half cycle	135.4	135.1	-0.3	±2.0
Negative half cycle	135.4	135.1	-0.3	±2.0

11. Overload indication

Measured value (dB)		Deviated Value (dB)	Acceptance Limits (dB)
Positive one-half cycle	Negative one-half cycle		
89.5	89.6	0.1	±1.5

12. High level stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor $k = 2$ or any value following calculation,providing a lavel of confidence of approximately 95 %

End of Calibration Certificate

SITHIPORN ASSOCIATES CO., LTD.
CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand
Tel. +66 2433 8331 Email : calibration@sithiphorn.com

NSC-TISI-TIS 17025
CALIBRATION 0394

Calibration Certificate

Equipment :	SOUND LEVEL METER
Manufacturer :	RION
Model :	NL-42 / Microphone UC-52 / Preamplifier NH-24
Serial No.:	01073423 / 169513 / 73684
ID No.:	RYG_FS0386

Condition As Found : GOOD

Customer : ALS LABORATORY GROUP (THAILAND) CO., LTD.
104 PHATTHANAKAN 40, PHATTHANAKAN ROAD,
KHWAENG PHATTHANAKAN, KHET SUAN LUANG,
BANGKOK, 10250 THAILAND.

Location :	-	
Ambient Temperature :	(23.0 ± 3)	°C
Pressure :	(101.3 ± 3)	kPa
Relative Humidity :	(50.0 ± 20)	%

REVIEW BY Nonakorn P.
APPROVED BY
NEXT CAL. DATE 9/10/25

Received Date :	23 SEPTEMBER 2024
Calibration Date :	09 OCTOBER 2024
Date of Issue :	09 OCTOBER 2024

Calibrated by : Nathakorn Pisutpaisan

Approved by :

(Thanakul Petchurai)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

SITHIPORN ASSOCIATES CO., LTD.
CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand
Tel. +66 2433 8331 Email : calibration@sithiphorn.com

SITHIPORN associates

NSC-TISI-TIS 17025
CALIBRATION 0394

Calibration Procedure : CP-AC-01

Calibration Method :

This equipment was calibrated by follow on IEC-61672-3 (2013) Standard for sound level meter (SLM).
The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.
For tests results of each items were made by observation of each Instruments display and also with SLM's display.

Condition of this result of calibration :

1. Reference Standard Instruments :

Instrument	Model	Serial No.	Cert. No.	Due Date
Waveform Generator	33210A	MY48017076	EF-0009-24	05-FEB-25
Waveform Generator	33511B	MY52302742	EF-0007-24	05-FEB-25
Digital Multimeter	33461A	MY53220104	EEL.BP 21/0267	13-FEB-25
Digital Multimeter	33461A	MY53220076	EEL.BP 20/0267	15-FEB-25
Digital Multimeter	34461A	MY60024273	EEL.BP 22/0267	15-FEB-25
Programmable Attenuator	MAT-1070	62100114	EF-0008-24	05-FEB-25
Condenser Microphone	4180	2977900	AA-1001-24	12-FEB-25
Measuring Amplifier	NA-42KAI	34560495	AA-3001-24	05-FEB-25

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.
3. This certificate is traceable to the international system of unit maintained at :
   - 3.1 National Institute of Metrology (Thailand).
   - 3.2 Thailand Institute of Scientific and Technological Research (TISTR).

SITHIPORN ASSOCIATES CO., LTD.
CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand
Tel. +66 2433 8331 Email : calibration@sithiphorn.com

SITHIPORN associates

NSC-TISI-TIS 17025
CALIBRATION 0394

Summary of Measurement Result :

Parameter	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	0.2	N/A
2. Self-generated noise	0.2	N/A
3. Acoustical signal tests of frequency weightings		
125 Hz	0.3	0.6
1000 Hz	0.3	0.6
8000 Hz	0.3	0.7
4. Electrical signal tests of frequency weightings		
For 10 Hz to 4 kHz	0.3	0.6
For > 4 kHz to 10 kHz	0.3	0.7
For > 10 kHz to 20 kHz	0.3	1.0
5. Frequency and time weightings at 1 kHz	0.2	0.2
6. Long - term stability	0.1	0.1
7. Level linearity on the reference level range	0.2	0.3
8. Level linearity including the level range control	0.2	0.3
9. Tone burst response	0.2	0.3
10. Peak C sound level	0.2	0.35
11. Overload indication	0.2	0.25
12. High level stability	0.1	0.1

SITHIPORN ASSOCIATES CO., LTD.
CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand
Tel. +66 2433 8331 Email : calibration@sithiphorn.com

SITHIPORN associates

NSC-TISI-TIS 17025
CALIBRATION 0394

Result of calibration :

1. Absolute sensitivity

Reference Acoustic Signal (dB)	Measured Value (dB)	Deviation (dB)	Acceptance Limit (dB)
93.9 (93.94)	93.9	0.0	±0.3

2. Self-generated noise

2.1 Normal test

Measured Value (dB)
15.7

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Weighting (dB)
A - weight	14.8
C - weight	21.2
Flat	26.6

3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
125	0.1	0.1	0.1	± 1.5
1000	0.0	0.0	0.0	± 1.0
8000	0.3	0.4	0.4	±5.0

SITHIPORN ASSOCIATES CO., LTD.
CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand
Tel. +66 2433 8331 Email : calibration@sithiphorn.com

SITHIPORN associates

NSC-TISI-TIS 17025
CALIBRATION 0394

4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	0.0	0.0	-0.1	±2.0
125	0.0	0.0	0.0	±1.5
250	0.0	0.0	0.0	±1.5
500	0.0	0.0	-0.1	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.0	0.0	±2.0
4000	0.0	0.0	0.0	±3.0
8000	0.0	0.1	0.1	±5.0

5. Frequency and time weightings at 1 kHz

5.1 Frequency weightings at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.2
C - weight	94.0	94.0	0.0	± 0.2
Flat	94.0	94.0	0.0	± 0.2

5.2 Time weighting at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	94.0	94.0	0.0	± 0.1
Slow	94.0	94.0	0.0	± 0.1
Leq	94.0	94.0	0.0	± 0.1

6. Long - term stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.3

SITHIPORN ASSOCIATES CO., LTD.
CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand
Tel. +66 2433 8331 Email : calibration@sithiphorn.com

SITHIPORN associates

NSC-TISI-TIS 17025
CALIBRATION 0394

7. Level linearity on the reference level range

Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
137.0	137.0	0.0	± 1.1
136.0	136.0	0.0	± 1.1
135.0	135.0	0.0	± 1.1
134.0	134.0	0.0	± 1.1
133.0	133.0	0.0	± 1.1
132.0	132.0	0.0	± 1.1
131.0	131.0	0.0	± 1.1
129.0	129.0	0.0	± 1.1
124.0	124.0	0.0	± 1.1
119.0	119.0	0.0	± 1.1
114.0	114.0	0.0	± 1.1
109.0	109.0	0.0	± 1.1
104.0	104.0	0.0	± 1.1
99.0	99.0	0.0	± 1.1
94.0	94.0	0.0	± 1.1
89.0	89.0	0.0	± 1.1
84.0	84.0	0.0	± 1.1
79.0	79.0	0.0	± 1.1
74.0	74.0	0.0	± 1.1
69.0	69.0	0.0	± 1.1
64.0	64.0	0.0	± 1.1
59.0	59.0	0.0	± 1.1
54.0	54.0	0.0	± 1.1
49.0	49.0	0.0	± 1.1
44.0	44.0	0.0	± 1.1
39.0	39.0	0.0	± 1.1
34.0	34.1	0.1	± 1.1
30.0	30.0	0.0	± 1.1
29.0	29.1	0.1	± 1.1
28.0	28.1	0.1	± 1.1
27.0	27.2	0.2	± 1.1
26.0	26.2	0.2	± 1.1
25.0	25.3	0.3	± 1.1

SITHIPORN ASSOCIATES CO., LTD.
CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand
Tel. +66 2433 8331 Email : calibration@sithiphorn.com

SITHIPORN associates

NSC-TISI-TIS 17025
CALIBRATION 0394

8. Level linearity including the level range control

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
130	94.0	94.0	0.0	±1.1

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
130	30.0	29.9	-0.1	±1.1

9. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Cycle	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.0	0.0	±1.0
Slow	2	8	108.0	108.0	0.0	1.5 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
SEL	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.0	0.0	±1.0

SITHIPORN ASSOCIATES CO., LTD.
CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand
Tel. +66 2433 8331 Email : calibration@sithiphorn.com

SITHIPORN associates

NSC-TISI-TIS 17025
CALIBRATION 0394

10. Peak C sound level

Number of cycle in test signal	Anticipated Value (dB)	Measured Value, Lcpeak (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	±3.0
One	136.4	136.3	-0.1	±3.0

Number of cycle in test signal	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	±2.0
Positive half cycle	135.4	135.2	-0.2	±2.0
Negative half cycle	135.4	135.2	-0.2	±2.0

11. Overload indication

Measured value (dB)		Deviated Value (dB)	Acceptance Limits (dB)
Positive one-half cycle	Negative one-half cycle		
89.5	89.5	0.0	±1.5

12. High level stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor $k = 2$ or any value following calculation,providing a lavel of confidence of approximately 95 %

End of Calibration Certificate

SITHIPORN ASSOCIATES CO., LTD.
CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand
Tel. +66 2433 8331 Email : calibration@sithiphorn.com

NSC-TISI-TIS 17025
CALIBRATION 0394

Calibration Certificate

Equipment :	SOUND LEVEL METER
Manufacturer :	RION
Model :	NL-42 / Microphone UC-52 / Preamplifier NH-24
Serial No.:	00472126 / 158778 / 88180
ID No.:	RYG_FS0301

Condition As Found : GOOD

Customer : ALS LABORATORY GROUP (THAILAND) CO., LTD.
104 PHATTHANAKAN 40, PHATTHANAKAN ROAD,
KHWAENG PHATTHANAKAN, KHET SUAN LUANG,
BANGKOK, 10250 THAILAND.

Location :	-	
Ambient Temperature :	(23.0 ± 3)	°C
Pressure :	(101.3 ± 3)	kPa
Relative Humidity :	(50.0 ± 20)	%

Received Date :	14 JANUARY 2025
Calibration Date :	27-29 JANUARY 2025
Date of Issue :	30 JANUARY 2025

REVIEW BY .....

APPROVED BY.....

NEXT CAL DATE.....26/ 01/ 2026.....

Calibrated by : Nathakorn Pisutpaisan

Approved by :

(Thanakul Petchurai)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

Cert. No. : ACL25100
Job No. : VC68AC0064
Pages : 2 of 8

Calibration Procedure : CP-AC-01

Calibration Method :

This equipment was calibrated by follow on IEC-61672-3 (2013) Standard for sound level meter (SLM).
The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.
For tests results of each items were made by observation of each Instruments display and also with SLM's display.

Condition of this result of calibration :

1. Reference Standard Instruments :

Instrument	Model	Serial No.	Cert. No.	Due Date
Waveform Generator	33210A	MY48017076	EF-0009-24	05-FEB-25
Waveform Generator	33511B	MY52302742	EF-0007-24	05-FEB-25
Digital Multimeter	33461A	MY53220104	EEL.BP 21/0267	13-FEB-25
Digital Multimeter	33461A	MY53220076	EEL.BP 20/0267	15-FEB-25
Digital Multimeter	34461A	MY60024273	EEL.BP 22/0267	15-FEB-25
Programmable Attenuator	MAT-1070	62100114	EF-0008-24	05-FEB-25
Condenser Microphone	4180	2977900	AA-1001-24	12-FEB-25
Measuring Amplifier	NA-42KAI	34560495	AA-3001-24	05-FEB-25

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.
3. This certificate is traceable to the international system of unit maintained at :
   - 3.1 National Institute of Metrology (Thailand).
   - 3.2 Thailand Institute of Scientific and Technological Research (TISTR).

Cert. No. : ACL25100
Job No. : VC68AC0064
Pages : 3 of 8

Summary of Measurement Result :

Parameter	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	0.2	N/A
2. Self-generated noise	0.2	N/A
3. Acoustical signal tests of frequency weightings		
125 Hz	0.3	0.6
1000 Hz	0.3	0.6
8000 Hz	0.3	0.7
4. Electrical signal tests of frequency weightings		
For 10 Hz to 4 kHz	0.3	0.6
For > 4 kHz to 10 kHz	0.3	0.7
For > 10 kHz to 20 kHz	0.3	1.0
5. Frequency and time weightings at 1 kHz	0.2	0.2
6. Long - term stability	0.1	0.1
7. Level linearity on the reference level range	0.2	0.3
8. Level linearity including the level range control	0.2	0.3
9. Tone burst response	0.2	0.3
10. Peak C sound level	0.2	0.35
11. Overload indication	0.2	0.25
12. High level stability	0.1	0.1

Cert. No. : **ACL25100**
Job No. : **VC68AC0064**
Page : **4 of 8**

Result of calibration :

1. Absolute sensitivity

Reference Acoustic Signal (dB)	Measured Value (dB)	Deviation (dB)	Acceptance Limit (dB)
93.9 (93.94)	93.9	0.0	±0.3

2. Self-generated noise

2.1 Normal test

Measured Value (dB)
13.6

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Weighting (dB)
A - weight	9.9
C - weight	16.4
Flat	22.2

3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
125	0.7	0.8	0.9	± 1.5
1000	0.1	0.1	0.1	± 1.0
8000	-3.2	-3.2	-3.8	±5.0

Cert. No. : ACL25100
Job No. : VC68AC0064
Pages : 5 of 8

4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	-0.1	0.0	0.0	±2.0
125	0.0	0.0	0.0	±1.5
250	0.0	0.0	-0.1	±1.5
500	0.0	0.0	-0.1	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.0	0.0	±2.0
4000	0.0	0.0	0.0	±3.0
8000	0.0	0.0	0.0	±5.0

5. Frequency and time weightings at 1 kHz

5.1 Frequency weightings at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.2
C - weight	94.0	94.0	0.0	± 0.2
Flat	94.0	94.0	0.0	± 0.2

5.2 Time weighting at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	94.0	94.0	0.0	± 0.1
Slow	94.0	94.0	0.0	± 0.1
Leq	94.0	94.0	0.0	± 0.1

6. Long - term stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.3

Cert. No. : ACL25100
Job No. : VC68AC0064
Pages : 6 of 8

7. Level linearity on the reference level range

Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
137.0	137.0	0.0	± 1.1
136.0	136.0	0.0	± 1.1
135.0	135.1	0.1	± 1.1
134.0	134.1	0.1	± 1.1
133.0	133.0	0.0	± 1.1
132.0	132.0	0.0	± 1.1
131.0	131.0	0.0	± 1.1
129.0	129.1	0.1	± 1.1
124.0	124.0	0.0	± 1.1
119.0	119.1	0.1	± 1.1
114.0	114.1	0.1	± 1.1
109.0	109.1	0.1	± 1.1
104.0	104.1	0.1	± 1.1
99.0	99.1	0.1	± 1.1
94.0	94.0	0.0	± 1.1
89.0	89.0	0.0	± 1.1
84.0	84.0	0.0	± 1.1
79.0	79.0	0.0	± 1.1
74.0	74.0	0.0	± 1.1
69.0	69.0	0.0	± 1.1
64.0	64.0	0.0	± 1.1
59.0	59.0	0.0	± 1.1
54.0	54.0	0.0	± 1.1
49.0	49.0	0.0	± 1.1
44.0	44.0	0.0	± 1.1
39.0	39.0	0.0	± 1.1
34.0	34.0	0.0	± 1.1
30.0	30.0	0.0	± 1.1
29.0	28.9	-0.1	± 1.1
28.0	28.0	0.0	± 1.1
27.0	27.0	0.0	± 1.1
26.0	26.0	0.0	± 1.1
25.0	25.0	0.0	± 1.1

8. Level linearity including the level range control

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
130	94.0	94.0	0.0	±1.1

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
130	29.0	29.0	0.0	±1.1

9. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Cycle	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	116.9	-0.1	1.0 ; -2.5
	200	800	134.0	134.0	0.0	±1.0
Slow	2	8	108.0	108.0	0.0	1.5 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
SEL	0.25	1	99.0	98.8	-0.2	1.5 ; -5.0
	2	8	108.0	107.9	-0.1	1.0 ; -2.5
	200	800	128.0	128.0	0.0	±1.0

Cert. No. : ACL25100
Job No. : VC68AC0064
Pages : 8 of 8

10. Peak C sound level

Number of cycle in test signal	Anticipated Value (dB)	Measured Value, Lcpeak (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	130.0	130.0	0.0	±3.0
One	133.4	133.4	0.0	±3.0

Number of cycle in test signal	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	±2.0
Positive half cycle	135.4	135.1	-0.3	±2.0
Negative half cycle	135.4	135.1	-0.3	±2.0

11. Overload indication

Measured value (dB)		Deviated Value (dB)	Acceptance Limits (dB)
Positive one-half cycle	Negative one-half cycle		
89.5	89.5	0.0	±1.5

12. High level stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor $k = 2$ or any value following calculation,providing a lavel of confidence of approximately 95 %

End of Calibration Certificate

SITHIPORN ASSOCIATES CO., LTD.
CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand
Tel. +66 2433 8331 Email : calibration@sithiphorn.com

NSC-TISI-TIS 17025
CALIBRATION 0394

Calibration Certificate

Equipment :	SOUND LEVEL METER
Manufacturer :	RION
Model :	NL-42 / Microphone UC-52 / Preamplifier NH-24
Serial No.:	00296515 / 179119 / 87526
ID No.:	RYG_FS0432

Condition As Found : GOOD

Customer : ALS LABORATORY GROUP (THAILAND) CO., LTD.
104 PHATTHANAKAN 40, PHATTHANAKAN ROAD,
KHWAENG PHATTHANAKAN, KHET SUAN LUANG,
BANGKOK, 10250 THAILAND.

Location :	-	
Ambient Temperature :	(23.0 ± 3)	°C
Pressure :	(101.3 ± 3)	kPa
Relative Humidity :	(50.0 ± 20)	%

Received Date :	14 JANUARY 2025
Calibration Date :	27-29 JANUARY 2025
Date of Issue :	30 JANUARY 2025

REVIEW BY .....

APPROVED BY.....

NEXT CAL DATE.....26/ 01/ 2026.....

Calibrated by : Nathakorn Pisutpaisan

Approved by :

(Thanakul Petchurai)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

Cert. No. : ACL25102
Job No. : VC68AC0064
Pages : 2 of 8

Calibration Procedure : CP-AC-01

Calibration Method :

This equipment was calibrated by follow on IEC-61672-3 (2013) Standard for sound level meter (SLM).
The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.
For tests results of each items were made by observation of each Instruments display and also with SLM's display.

Condition of this result of calibration :

1. Reference Standard Instruments :

Instrument	Model	Serial No.	Cert. No.	Due Date
Waveform Generator	33210A	MY48017076	EF-0009-24	05-FEB-25
Waveform Generator	33511B	MY52302742	EF-0007-24	05-FEB-25
Digital Multimeter	33461A	MY53220104	EEL.BP 21/0267	13-FEB-25
Digital Multimeter	33461A	MY53220076	EEL.BP 20/0267	15-FEB-25
Digital Multimeter	34461A	MY60024273	EEL.BP 22/0267	15-FEB-25
Programmable Attenuator	MAT-1070	62100114	EF-0008-24	05-FEB-25
Condenser Microphone	4180	2977900	AA-1001-24	12-FEB-25
Measuring Amplifier	NA-42KAI	34560495	AA-3001-24	05-FEB-25

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.
3. This certificate is traceable to the international system of unit maintained at :
   - 3.1 National Institute of Metrology (Thailand).
   - 3.2 Thailand Institute of Scientific and Technological Research (TISTR).

Cert. No. : ACL25102
Job No. : VC68AC0064
Pages : 3 of 8

Summary of Measurement Result :

Parameter	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	0.2	N/A
2. Self-generated noise	0.2	N/A
3. Acoustical signal tests of frequency weightings		
125 Hz	0.3	0.6
1000 Hz	0.3	0.6
8000 Hz	0.3	0.7
4. Electrical signal tests of frequency weightings		
For 10 Hz to 4 kHz	0.3	0.6
For > 4 kHz to 10 kHz	0.3	0.7
For > 10 kHz to 20 kHz	0.3	1.0
5. Frequency and time weightings at 1 kHz	0.2	0.2
6. Long - term stability	0.1	0.1
7. Level linearity on the reference level range	0.2	0.3
8. Level linearity including the level range control	0.2	0.3
9. Tone burst response	0.2	0.3
10. Peak C sound level	0.2	0.35
11. Overload indication	0.2	0.25
12. High level stability	0.1	0.1

Cert. No. : **ACL25102**
Job No. : **VC68AC0064**
Page : **4 of 8**

Result of calibration :

1. Absolute sensitivity

Reference Acoustic Signal (dB)	Measured Value (dB)	Deviation (dB)	Acceptance Limit (dB)
93.9 (93.94)	93.9	0.0	±0.3

2. Self-generated noise

2.1 Normal test

Measured Value (dB)
14.2

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Weighting (dB)
A - weight	10.8
C - weight	17.3
Flat	23.0

3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
125	0.2	0.2	0.2	± 1.5
1000	0.0	0.0	0.0	± 1.0
8000	0.2	0.2	0.2	±5.0

Cert. No. : ACL25102
Job No. : VC68AC0064
Pages : 5 of 8

4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	-0.1	-0.1	-0.1	±2.0
125	0.0	0.0	0.0	±1.5
250	0.0	0.0	0.0	±1.5
500	0.0	0.0	0.0	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.0	0.0	±2.0
4000	0.0	0.0	0.0	±3.0
8000	0.0	0.1	0.1	±5.0

5. Frequency and time weightings at 1 kHz

5.1 Frequency weightings at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.2
C - weight	94.0	94.0	0.0	± 0.2
Flat	94.0	94.0	0.0	± 0.2

5.2 Time weighting at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	94.0	94.0	0.0	± 0.1
Slow	94.0	94.0	0.0	± 0.1
Leq	94.0	94.0	0.0	± 0.1

6. Long - term stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.3

Cert. No. : ACL25102
Job No. : VC68AC0064
Pages : 6 of 8

7. Level linearity on the reference level range

Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
137.0	137.0	0.0	± 1.1
136.0	136.0	0.0	± 1.1
135.0	135.0	0.0	± 1.1
134.0	134.0	0.0	± 1.1
133.0	133.0	0.0	± 1.1
132.0	132.0	0.0	± 1.1
131.0	131.0	0.0	± 1.1
129.0	129.0	0.0	± 1.1
124.0	124.0	0.0	± 1.1
119.0	119.0	0.0	± 1.1
114.0	114.0	0.0	± 1.1
109.0	109.0	0.0	± 1.1
104.0	104.0	0.0	± 1.1
99.0	99.0	0.0	± 1.1
94.0	94.0	0.0	± 1.1
89.0	89.0	0.0	± 1.1
84.0	84.0	0.0	± 1.1
79.0	79.0	0.0	± 1.1
74.0	74.0	0.0	± 1.1
69.0	69.0	0.0	± 1.1
64.0	64.0	0.0	± 1.1
59.0	59.0	0.0	± 1.1
54.0	53.9	-0.1	± 1.1
49.0	49.0	0.0	± 1.1
44.0	44.0	0.0	± 1.1
39.0	38.9	-0.1	± 1.1
34.0	33.9	-0.1	± 1.1
30.0	29.9	-0.1	± 1.1
29.0	28.9	-0.1	± 1.1
28.0	27.9	-0.1	± 1.1
27.0	26.9	-0.1	± 1.1
26.0	25.9	-0.1	± 1.1
25.0	24.9	-0.1	± 1.1

Cert. No. : ACL25102
Job No. : VC68AC0064
Pages : 7 of 8

8. Level linearity including the level range control

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
130	94.0	94.0	0.0	±1.1

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
130	29.0	28.8	-0.2	±1.1

9. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Cycle	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.0	0.0	±1.0
Slow	2	8	108.0	108.0	0.0	1.5 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
SEL	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.0	0.0	±1.0

10. Peak C sound level

Number of cycle in test signal	Anticipated Value (dB)	Measured Value, Lcpeak (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	130.0	130.0	0.0	±3.0
One	133.4	133.3	-0.1	±3.0

Number of cycle in test signal	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	±2.0
Positive half cycle	135.4	135.2	-0.2	±2.0
Negative half cycle	135.4	135.2	-0.2	±2.0

11. Overload indication

Measured value (dB)		Deviated Value (dB)	Acceptance Limits (dB)
Positive one-half cycle	Negative one-half cycle		
89.5	89.5	0.0	±1.5

12. High level stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor $k = 2$ or any value following calculation,providing a lavel of confidence of approximately 95 %

End of Calibration Certificate

SITHIPORN ASSOCIATES CO., LTD.
CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand
Tel. +66 2433 8331 Email : calibration@sithiphorn.com

SITHIPORN associates

NSC-TISI-TIS 17025
CALIBRATION 0394

Calibration Certificate

Equipment :	SOUND LEVEL METER
Manufacturer :	RION
Model :	NL-42 / Microphone UC-52 / Preamplifier NH-24
Serial No.:	00296516 / 180412 / 88182
ID No.:	RYG_FS0433

Condition As Found : GOOD

Customer : ALS LABORATORY GROUP (THAILAND) CO., LTD.
104 PHATTHANAKAN 40, PHATTHANAKAN ROAD,
KHWAENG PHATTHANAKAN, KHET SUAN LUANG,
BANGKOK, 10250 THAILAND.

Location :	-	
Ambient Temperature :	(23.0 ±3)	°C
Pressure :	(101.3 ±3)	kPa
Relative Humidity :	(50.0 ±20)	%

Received Date : 14 JANUARY 2025
Calibration Date : 27-29 JANUARY 2025
Date of Issue : 30 JANUARY 2025

REVIEW BY .....

APPROVED BY.....

NEXT CAL DATE 26/ 01/ 2026.....

Calibrated by : Nathakorn Pisutpaisan

Approved by :

(Thanakul Petchurai)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

Cert. No. : ACL25103
Job No. : VC68AC0064
Pages : 2 of 8

Calibration Procedure : CP-AC-01

Calibration Method :

This equipment was calibrated by follow on IEC-61672-3 (2013) Standard for sound level meter (SLM).
The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.
For tests results of each items were made by observation of each Instruments display and also with SLM's display.

Condition of this result of calibration :

1. Reference Standard Instruments :

Instrument	Model	Serial No.	Cert. No.	Due Date
Waveform Generator	33210A	MY48017076	EF-0009-24	05-FEB-25
Waveform Generator	33511B	MY52302742	EF-0007-24	05-FEB-25
Digital Multimeter	33461A	MY53220104	EEL.BP 21/0267	13-FEB-25
Digital Multimeter	33461A	MY53220076	EEL.BP 20/0267	15-FEB-25
Digital Multimeter	34461A	MY60024273	EEL.BP 22/0267	15-FEB-25
Programmable Attenuator	MAT-1070	62100114	EF-0008-24	05-FEB-25
Condenser Microphone	4180	2977900	AA-1001-24	12-FEB-25
Measuring Amplifier	NA-42KAI	34560495	AA-3001-24	05-FEB-25

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.
3. This certificate is traceable to the international system of unit maintained at :
   - 3.1 National Institute of Metrology (Thailand).
   - 3.2 Thailand Institute of Scientific and Technological Research (TISTR).

Cert. No. : ACL25103
Job No. : VC68AC0064
Pages : 3 of 8

Summary of Measurement Result :

Parameter	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	0.2	N/A
2. Self-generated noise	0.2	N/A
3. Acoustical signal tests of frequency weightings		
125 Hz	0.3	0.6
1000 Hz	0.3	0.6
8000 Hz	0.3	0.7
4. Electrical signal tests of frequency weightings		
For 10 Hz to 4 kHz	0.3	0.6
For > 4 kHz to 10 kHz	0.3	0.7
For > 10 kHz to 20 kHz	0.3	1.0
5. Frequency and time weightings at 1 kHz	0.2	0.2
6. Long - term stability	0.1	0.1
7. Level linearity on the reference level range	0.2	0.3
8. Level linearity including the level range control	0.2	0.3
9. Tone burst response	0.2	0.3
10. Peak C sound level	0.2	0.35
11. Overload indication	0.2	0.25
12. High level stability	0.1	0.1

Cert. No. : ACL25103
Job No. : VC68AC0064
Page : 4 of 8

Result of calibration :

1. Absolute sensitivity

Reference Acoustic Signal (dB)	Measured Value (dB)	Deviation (dB)	Acceptance Limit (dB)
93.9 (93.94)	93.9	0.0	±0.3

2. Self-generated noise

2.1 Normal test

Measured Value (dB)
14.2

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Weighting (dB)
A - weight	10.8
C - weight	17.3
Flat	22.9

3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
125	0.3	0.3	0.3	± 1.5
1000	0.0	0.0	0.0	± 1.0
8000	1.0	1.0	1.0	±5.0

Cert. No. : ACL25103
Job No. : VC68AC0064
Pages : 5 of 8

4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	0.0	-0.1	0.0	±2.0
125	0.0	0.0	0.0	±1.5
250	0.0	0.0	-0.1	±1.5
500	0.0	0.0	-0.1	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.0	0.0	±2.0
4000	0.0	0.0	0.0	±3.0
8000	0.0	0.1	0.1	±5.0

5. Frequency and time weightings at 1 kHz

5.1 Frequency weightings at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.2
C - weight	94.0	94.0	0.0	± 0.2
Flat	94.0	94.0	0.0	± 0.2

5.2 Time weighting at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	94.0	94.0	0.0	± 0.1
Slow	94.0	94.0	0.0	± 0.1
Leq	94.0	94.0	0.0	± 0.1

6. Long - term stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.3

Cert. No. : ACL25103
Job No. : VC68AC0064
Pages : 6 of 8

7. Level linearity on the reference level range

Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
137.0	137.0	0.0	± 1.1
136.0	136.0	0.0	± 1.1
135.0	135.0	0.0	± 1.1
134.0	134.0	0.0	± 1.1
133.0	132.9	-0.1	± 1.1
132.0	131.9	-0.1	± 1.1
131.0	130.9	-0.1	± 1.1
129.0	129.0	0.0	± 1.1
124.0	124.0	0.0	± 1.1
119.0	119.0	0.0	± 1.1
114.0	114.0	0.0	± 1.1
109.0	109.0	0.0	± 1.1
104.0	104.0	0.0	± 1.1
99.0	99.0	0.0	± 1.1
94.0	94.0	0.0	± 1.1
89.0	89.0	0.0	± 1.1
84.0	84.0	0.0	± 1.1
79.0	79.0	0.0	± 1.1
74.0	74.0	0.0	± 1.1
69.0	69.0	0.0	± 1.1
64.0	64.0	0.0	± 1.1
59.0	59.0	0.0	± 1.1
54.0	54.0	0.0	± 1.1
49.0	49.0	0.0	± 1.1
44.0	44.0	0.0	± 1.1
39.0	39.0	0.0	± 1.1
34.0	34.0	0.0	± 1.1
30.0	29.9	-0.1	± 1.1
29.0	28.9	-0.1	± 1.1
28.0	27.9	-0.1	± 1.1
27.0	26.9	-0.1	± 1.1
26.0	25.9	-0.1	± 1.1
25.0	24.8	-0.2	± 1.1

Cert. No. : ACL25103
Job No. : VC68AC0064
Pages : 7 of 8

8. Level linearity including the level range control

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
130	94.0	94.0	0.0	±1.1

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
130	29.0	28.9	-0.1	±1.1

9. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Cycle	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.0	0.0	±1.0
Slow	2	8	108.0	108.0	0.0	1.5 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
SEL	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.0	0.0	±1.0

Cert. No. : ACL25103
Job No. : VC68AC0064
Pages : 8 of 8

10. Peak C sound level

Number of cycle in test signal	Anticipated Value (dB)	Measured Value, Lcpeak (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	130.0	130.0	0.0	±3.0
One	133.4	133.4	0.0	±3.0

Number of cycle in test signal	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	±2.0
Positive half cycle	135.4	135.1	-0.3	±2.0
Negative half cycle	135.4	135.2	-0.2	±2.0

11. Overload indication

Measured value (dB)		Deviated Value (dB)	Acceptance Limits (dB)
Positive one-half cycle	Negative one-half cycle		
89.5	89.5	0.0	±1.5

12. High level stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor $k = 2$ or any value following calculation,providing a lavel of confidence of approximately 95 %

End of Calibration Certificate

SITHIPORN ASSOCIATES CO., LTD.
CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand
Tel. +66 2433 8331 Email : calibration@sithiphorn.com

NSC-TISI-TIS 17025
CALIBRATION 0394

Cert. No. : ACL25104
Pages : 1 of 8

Calibration Certificate

Equipment :	SOUND LEVEL METER
Manufacturer :	RION
Model :	NL-42 / Microphone UC-52 / Preamplifier NH-24
Serial No.:	00296517 / 135220 / 87527
ID No.:	RYG_FS0434

Condition As Found : GOOD

Customer : ALS LABORATORY GROUP (THAILAND) CO., LTD.
104 PHATTHANAKAN 40, PHATTHANAKAN ROAD,
KHWAENG PHATTHANAKAN, KHET SUAN LUANG,
BANGKOK, 10250 THAILAND.

Location :	-	
Ambient Temperature :	(23.0 ±3)	°C
Pressure :	(101.3 ±3)	kPa
Relative Humidity :	(50.0 ±20)	%

Received Date :	14 JANUARY 2025
Calibration Date :	27-29 JANUARY 2025
Date of Issue :	30 JANUARY 2025

REVIEW BY .....

APPROVED BY.....

NEXT CAL DATE.....26/ 01/ 2026.....

Calibrated by : Nathakorn Pisutpaisan

Approved by :

(Thanakul Petchurai)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

Cert. No. : ACL25104
Job No. : VC68AC0064
Pages : 2 of 8

Calibration Procedure : CP-AC-01

Calibration Method :

This equipment was calibrated by follow on IEC-61672-3 (2013) Standard for sound level meter (SLM).
The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.
For tests results of each items were made by observation of each Instruments display and also with SLM's display.

Condition of this result of calibration :

1. Reference Standard Instruments :

Instrument	Model	Serial No.	Cert. No.	Due Date
Waveform Generator	33210A	MY48017076	EF-0009-24	05-FEB-25
Waveform Generator	33511B	MY52302742	EF-0007-24	05-FEB-25
Digital Multimeter	33461A	MY53220104	EEL.BP 21/0267	13-FEB-25
Digital Multimeter	33461A	MY53220076	EEL.BP 20/0267	15-FEB-25
Digital Multimeter	34461A	MY60024273	EEL.BP 22/0267	15-FEB-25
Programmable Attenuator	MAT-1070	62100114	EF-0008-24	05-FEB-25
Condenser Microphone	4180	2977900	AA-1001-24	12-FEB-25
Measuring Amplifier	NA-42KAI	34560495	AA-3001-24	05-FEB-25

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.
3. This certificate is traceable to the international system of unit maintained at :
   - 3.1 National Institute of Metrology (Thailand).
   - 3.2 Thailand Institute of Scientific and Technological Research (TISTR).

Cert. No. : ACL25104
Job No. : VC68AC0064
Pages : 3 of 8

Summary of Measurement Result :

Parameter	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	0.2	N/A
2. Self-generated noise	0.2	N/A
3. Acoustical signal tests of frequency weightings		
125 Hz	0.3	0.6
1000 Hz	0.3	0.6
8000 Hz	0.3	0.7
4. Electrical signal tests of frequency weightings		
For 10 Hz to 4 kHz	0.3	0.6
For > 4 kHz to 10 kHz	0.3	0.7
For > 10 kHz to 20 kHz	0.3	1.0
5. Frequency and time weightings at 1 kHz	0.2	0.2
6. Long - term stability	0.1	0.1
7. Level linearity on the reference level range	0.2	0.3
8. Level linearity including the level range control	0.2	0.3
9. Tone burst response	0.2	0.3
10. Peak C sound level	0.2	0.35
11. Overload indication	0.2	0.25
12. High level stability	0.1	0.1

Cert. No. : ACL25104
Job No. : VC68AC0064

Result of calibration :

1. Absolute sensitivity

Reference Acoustic Signal (dB)	Measured Value (dB)	Deviation (dB)	Acceptance Limit (dB)
93.9 (93.94)	93.9	0.0	±0.3

2. Self-generated noise

2.1 Normal test

Measured Value (dB)
17.2

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Weighting (dB)
A - weight	14.6
C - weight	20.5
Flat	26.1

3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
125	-0.1	-0.1	-0.1	± 1.5
1000	-0.2	-0.2	-0.2	± 1.0
8000	0.2	0.2	0.2	±5.0

Cert. No. : ACL25104
Job No. : VC68AC0064
Pages : 5 of 8

4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	-0.1	0.0	0.0	±2.0
125	0.0	0.0	0.0	±1.5
250	0.0	0.0	0.0	±1.5
500	0.0	0.0	0.0	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.0	0.0	±2.0
4000	0.0	0.0	0.0	±3.0
8000	0.0	0.1	0.1	±5.0

5. Frequency and time weightings at 1 kHz

5.1 Frequency weightings at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.2
C - weight	94.0	94.0	0.0	± 0.2
Flat	94.0	94.0	0.0	± 0.2

5.2 Time weighting at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	94.0	94.0	0.0	± 0.1
Slow	94.0	94.0	0.0	± 0.1
Leq	94.0	94.0	0.0	± 0.1

6. Long - term stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.3

Cert. No. : ACL25104
Job No. : VC68AC0064
Pages : 6 of 8

7. Level linearity on the reference level range

Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
137.0	137.0	0.0	± 1.1
136.0	136.0	0.0	± 1.1
135.0	135.0	0.0	± 1.1
134.0	134.0	0.0	± 1.1
133.0	133.0	0.0	± 1.1
132.0	132.0	0.0	± 1.1
131.0	131.0	0.0	± 1.1
129.0	129.0	0.0	± 1.1
124.0	124.0	0.0	± 1.1
119.0	119.0	0.0	± 1.1
114.0	114.0	0.0	± 1.1
109.0	109.0	0.0	± 1.1
104.0	104.0	0.0	± 1.1
99.0	99.0	0.0	± 1.1
94.0	94.0	0.0	± 1.1
89.0	89.0	0.0	± 1.1
84.0	84.0	0.0	± 1.1
79.0	79.0	0.0	± 1.1
74.0	74.0	0.0	± 1.1
69.0	69.0	0.0	± 1.1
64.0	63.9	-0.1	± 1.1
59.0	59.0	0.0	± 1.1
54.0	53.9	-0.1	± 1.1
49.0	48.9	-0.1	± 1.1
44.0	43.9	-0.1	± 1.1
39.0	38.9	-0.1	± 1.1
34.0	33.9	-0.1	± 1.1
30.0	29.9	-0.1	± 1.1
29.0	28.9	-0.1	± 1.1
28.0	27.9	-0.1	± 1.1
27.0	26.9	-0.1	± 1.1
26.0	25.9	-0.1	± 1.1
25.0	24.8	-0.2	± 1.1

Cert. No. : ACL25104
Job No. : VC68AC0064
Pages : 7 of 8

8. Level linearity including the level range control

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
130	94.0	94.0	0.0	±1.1

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
130	29.0	28.9	-0.1	±1.1

9. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Cycle	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.0	0.0	±1.0
Slow	2	8	108.0	108.0	0.0	1.5 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
SEL	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.0	0.0	±1.0

10. Peak C sound level

Number of cycle in test signal	Anticipated Value (dB)	Measured Value, Lcpeak (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	130.0	130.0	0.0	±3.0
One	133.4	133.3	-0.1	±3.0

Number of cycle in test signal	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	±2.0
Positive half cycle	135.4	135.2	-0.2	±2.0
Negative half cycle	135.4	135.2	-0.2	±2.0

11. Overload indication

Measured value (dB)		Deviated Value (dB)	Acceptance Limits (dB)
Positive one-half cycle	Negative one-half cycle		
89.5	89.6	0.1	±1.5

12. High level stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor $k = 2$ or any value following calculation,providing a lavel of confidence of approximately 95 %

End of Calibration Certificate

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7/139 MOO 13, SOI SUNTINAKORN 11 TAMBON BANG KAEO,
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL: (66)0-2116-5860-1 FAX:(66)0-2116-7140

ANSI National Accreditation Board ACCREDITED ISO/IEC 17025 CALIBRATION LABORATORY AC-2961

Certificate of Calibration

Customer

Name : ALS Laboratory Group Thailand Co., Ltd.

Address : 104 Soi Phatthanakan 40, Phatthanakan Road, Suan Luang, Bangkok 10250

Certificate No : 25-ACT-042

Request No : Req-2025-0604

Unit Under Calibration Details

Measurement item : Acoustic Calibrator

Manufacturer : RION

Model : NC-75

Serial Number : 35002736

ID : RYG_FS0496

Class : 1

Range : 94 dB / 1000 Hz

Instrument Status : Used

REVIEW BY ..... Narakorn P.

APPROVED BY .....

NEXT CAL DATE..... 19/03/26

Calibration Environment and Details

Temperature : (23 ±2 °C)

Humidity : (50 ± 20 %RH)

Barometric Pressure : (1013 ±10.0 hPa)

Received Date : 6 March 2025

Calibration Date : 19 March 2025

Location of Calibration : LAB 1 Acoustic

Calibration Procedure : In-house method CP-ACT-02 based on IEC 60942:2017 Electroacoustics - Sound calibrators

Reference Standard	Model	Serial Number	Traceable	Due Calibration
Sound Calibrator	SV 35A	58079	EEI	12 June 2025
THD Multimeter	2015	1047765	NIMT	4 February 2026

Traceability : This certificate providoes traceability of measurement to recognized national standard, and to the realization of the international System of Units (SI).

Note

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor k =2, providing a level of confidence approximately 95 %.

Calibrated By : Mr. Noppadon Luangart
Service Calibration Engineer

Approved By : Mr. Pacit Mathavorn
Calibration Engineer Supervisor

Issue Date : 19 March 2025

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7/139 MOO 13, SOI SUNTINAKORN 11 TAMBON BANG KAEO,
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL: (66)0-2116-5860-1 FAX: (66)0-2116-7140

Certificate No : 25-ACT-042

Request No : Req-2025-0604

Sound pressure level **Calibration Results :** Without Adjustment

Calibration Range (dB)	Without Adjustment (dB)		Adjustment (dB)		Uncertainty (± dB)	Acceptance limit Class 1 (± dB)	Result
	Measured	Deviated value	Measured	Deviated value			
94 dB / 1000 Hz	94.06	0.06	-	-	0.13	0.25	Pass

Frequency of Sound pressure level

Calibration Range (Hz)	Without Adjustment		Adjustment		Uncertainty (± %)	Acceptance limit Class 1 (± %)	Result
	Measured (Hz)	Deviated	Measured (Hz)	Deviated			
94 dB / 1000 Hz	1000.00	0.00	-	-	0.01	0.70	Pass

Total Harmonic Distortion plus Noise of Sound pressure level (THD+N %)

Calibration Range (Hz)	Without Adjustment	Adjustment	Uncertainty (± %)	Acceptance limit Class 1 (± %)	Result
	Measured (%)	Measured (%)			
94 dB / 1000 Hz	0.98	-	0.40	2.5	Pass

Note :

Function	Maximum-permitted Uncertainty of measurement
Sound pressure level	0.15 dB
Frequency	0.20%
Total distortion+noise	0.50%

- Acceptance limit was IEC60942:2017 Class 1
- The calibration results exclude the calibrator pressure correction
- The calibration results exclude the microphone volume correction

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7/139 MOO 13, SOI SUNTINAKORN 11 TAMBON BANG KAEO,
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL: (66)0-2116-5860-1 FAX: (66)0-2116-7140

Certificate No : 25-ACT-042

Request No : Req-2025-0604

Decision Rule for Statements of Conformity

The standard decision rule employed for the statements of conformity to each calibration result will be applied using ILAC-G8:09/2019; Guidelines on the Reporting of Compliance with Specification as following Fig. and statements

Pass = The measurement result plus the expanded uncertainty with a 95% coverage probability were within the limit.

Pass[1] = The measurement result was within the limit. However, a portion of the expanded uncertainty of measurement at 95% exceeds the limit.

Fail[1] = The measurement result was out of the limit. However, a portion of the expanded uncertainty of measurement at 95% is within the limit.

Fail = The measurement result plus the expanded uncertainty with a 95% coverage probability were outside the limit.

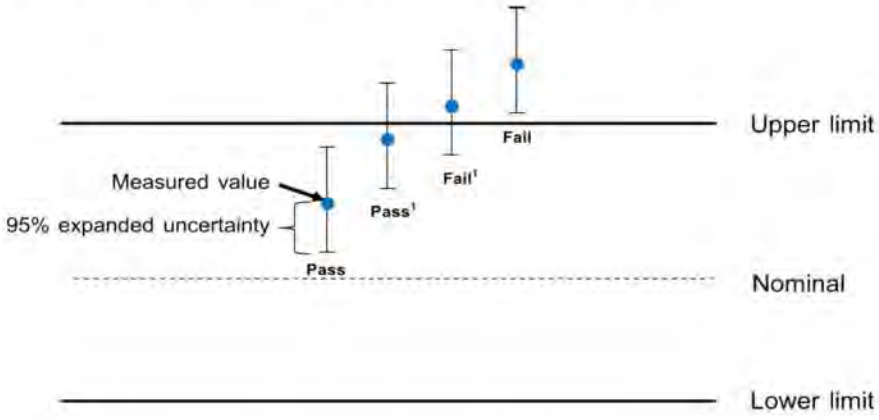

End of Calibration

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

SITHIPORN ASSOCIATES CO., LTD.
CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand
Tel. +66 2433 8331 Email : calibration@sithiphorn.com

NSC-TISI-TIS 17025
CALIBRATION 0394

Cert. No. : ACL25071
Pages : 1 of 8

Calibration Certificate

Equipment :	SOUND LEVEL METER
Manufacturer :	RION
Model :	NL-42 / Microphone UC-52 / Preamplifier NH-24
Serial No.:	01122579 / 172172 / 74022
ID No.:	RYG_FS0018

Condition As Found : GOOD

Customer : ALS LABORATORY GROUP (THAILAND) CO., LTD.
104 PHATTHANAKAN 40, PHATTHANAKAN ROAD,
KHWAENG PHATTHANAKAN, KHET SUAN LUANG,
BANGKOK, 10250 THAILAND.

Location :	-	
Ambient Temperature :	(23.0 ±3)	°C
Pressure :	(101.3 ±3)	kPa
Relative Humidity :	(50.0 ±20)	%

Received Date :	07 JANUARY 2025
Calibration Date :	21 - 23 JANUARY 2025
Date of Issue :	24 JANUARY 2025

REVIEW BY .....

APPROVED BY .....

NEXT CAL DATE..... 21/ 01/ 2026

Calibrated by : Nathakorn Pisutpaisan

Approved by :

(Thanakul Petchurai)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

Cert. No. : ACL25071
Job No. : VC68AC0059
Pages : 2 of 8

Calibration Procedure : CP-AC-01

Calibration Method :

This equipment was calibrated by follow on IEC-61672-3 (2013) Standard for sound level meter (SLM).

The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.

For tests results of each items were made by observation of each Instruments display and also with SLM's display.

Condition of this result of calibration :

1. Reference Standard Instruments :

Instrument	Model	Serial No.	Cert. No.	Due Date
Waveform Generator	33210A	MY48017076	EF-0009-24	05-FEB-25
Waveform Generator	33511B	MY52302742	EF-0007-24	05-FEB-25
Digital Multimeter	33461A	MY53220104	EEL.BP 21/0267	13-FEB-25
Digital Multimeter	33461A	MY53220076	EEL.BP 20/0267	15-FEB-25
Digital Multimeter	34461A	MY60024273	EEL.BP 22/0267	15-FEB-25
Programmable Attenuator	MAT-1070	62100114	EF-0008-24	05-FEB-25
Condenser Microphone	4180	2977900	AA-1001-24	12-FEB-25
Measuring Amplifier	NA-42KAI	34560495	AA-3001-24	05-FEB-25

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is traceable to the international system of unit maintained at :

3.1 National Institute of Metrology (Thailand).

3.2 Thailand Institute of Scientific and Technological Research (TISTR).

Cert. No. : ACL25071
Job No. : VC68AC0059
Pages : 3 of 8

Summary of Measurement Result :

Parameter	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	0.2	N/A
2. Self-generated noise	0.2	N/A
3. Acoustical signal tests of frequency weightings		
125 Hz	0.3	0.6
1000 Hz	0.3	0.6
8000 Hz	0.3	0.7
4. Electrical signal tests of frequency weightings		
For 10 Hz to 4 kHz	0.3	0.6
For > 4 kHz to 10 kHz	0.3	0.7
For > 10 kHz to 20 kHz	0.3	1.0
5. Frequency and time weightings at 1 kHz	0.2	0.2
6. Long - term stability	0.1	0.1
7. Level linearity on the reference level range	0.2	0.3
8. Level linearity including the level range control	0.2	0.3
9. Tone burst response	0.2	0.3
10. Peak C sound level	0.2	0.35
11. Overload indication	0.2	0.25
12. High level stability	0.1	0.1

Cert. No. : ACL25071
Job No. : VC68AC0059
Page : 4 of 8

Result of calibration :

1. Absolute sensitivity

Reference Acoustic Signal (dB)	Measured Value (dB)	Deviation (dB)	Acceptance Limit (dB)
93.9 (93.94)	93.9	0.0	±0.3

2. Self-generated noise

2.1 Normal test

Measured Value (dB)
14.8

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Weighting (dB)
A - weight	12.0
C - weight	18.3
Flat	24.0

3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
125	0.3	0.3	0.3	± 1.5
1000	0.1	0.1	0.1	± 1.0
8000	1.1	1.1	1.1	±5.0

Cert. No. : ACL25071
Job No. : VC68AC0059
Pages : 5 of 8

4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	0.0	0.0	0.0	±2.0
125	0.0	0.0	0.0	±1.5
250	0.0	0.0	0.0	±1.5
500	0.0	0.0	0.0	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.0	0.0	±2.0
4000	0.0	0.0	0.0	±3.0
8000	0.0	0.1	0.1	±5.0

5. Frequency and time weightings at 1 kHz

5.1 Frequency weightings at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.2
C - weight	94.0	94.0	0.0	± 0.2
Flat	94.0	94.0	0.0	± 0.2

5.2 Time weighting at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	94.0	94.0	0.0	± 0.1
Slow	94.0	94.0	0.0	± 0.1
Leq	94.0	94.0	0.0	± 0.1

6. Long - term stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.3

Cert. No. : ACL25071
Job No. : VC68AC0059
Pages : 6 of 8

7. Level linearity on the reference level range

Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
137.0	137.0	0.0	± 1.1
136.0	136.0	0.0	± 1.1
135.0	135.0	0.0	± 1.1
134.0	134.0	0.0	± 1.1
133.0	133.0	0.0	± 1.1
132.0	132.0	0.0	± 1.1
131.0	131.0	0.0	± 1.1
129.0	129.0	0.0	± 1.1
124.0	124.0	0.0	± 1.1
119.0	119.0	0.0	± 1.1
114.0	114.0	0.0	± 1.1
109.0	109.0	0.0	± 1.1
104.0	104.0	0.0	± 1.1
99.0	99.0	0.0	± 1.1
94.0	94.0	0.0	± 1.1
89.0	89.0	0.0	± 1.1
84.0	84.0	0.0	± 1.1
79.0	78.9	-0.1	± 1.1
74.0	74.0	0.0	± 1.1
69.0	69.0	0.0	± 1.1
64.0	63.9	-0.1	± 1.1
59.0	59.0	0.0	± 1.1
54.0	53.9	-0.1	± 1.1
49.0	48.9	-0.1	± 1.1
44.0	43.9	-0.1	± 1.1
39.0	38.9	-0.1	± 1.1
34.0	33.9	-0.1	± 1.1
30.0	30.0	0.0	± 1.1
29.0	28.9	-0.1	± 1.1
28.0	28.0	0.0	± 1.1
27.0	27.0	0.0	± 1.1
26.0	26.0	0.0	± 1.1
25.0	25.1	0.1	± 1.1

T. Retch.

Cert. No. : ACL25071
Job No. : VC68AC0059
Pages : 7 of 8

8. Level linearity including the level range control

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
130	94.0	94.0	0.0	±1.1

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
130	29.0	29.0	0.0	±1.1

9. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Cycle	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.0	0.0	±1.0
Slow	2	8	108.0	108.0	0.0	1.5 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
SEL	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.1	0.1	±1.0

Cert. No. : ACL25071
Job No. : VC68AC0059
Pages : 8 of 8

10. Peak C sound level

Number of cycle in test signal	Anticipated Value (dB)	Measured Value, Lcpeak (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	130.0	130.0	0.0	±3.0
One	133.4	133.3	-0.1	±3.0

Number of cycle in test signal	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	±2.0
Positive half cycle	135.4	135.2	-0.2	±2.0
Negative half cycle	135.4	135.2	-0.2	±2.0

11. Overload indication

Measured value (dB)		Deviated Value (dB)	Acceptance Limits (dB)
Positive one-half cycle	Negative one-half cycle		
89.5	89.6	0.1	±1.5

12. High level stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor $k = 2$ or any value following calculation,providing a lavel of confidence of approximately 95 %

End of Calibration Certificate

SITHIPORN ASSOCIATES CO., LTD.
CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand
Tel. +66 2433 8331 Email : calibration@sithiphorn.com

NSC-TISI-TIS 17025
CALIBRATION 0394

Cert. No. : ACL25072
Pages : 1 of 8

Calibration Certificate

Equipment :	SOUND LEVEL METER
Manufacturer :	RION
Model :	NL-42 / Microphone UC-52 / Preamplifier NH-24
Serial No.:	01122607 / 145554 / 34373
ID No.:	RYG_FS0019

Condition As Found : GOOD

Customer : ALS LABORATORY GROUP (THAILAND) CO., LTD.
104 PHATTHANAKAN 40, PHATTHANAKAN ROAD,
KHWAENG PHATTHANAKAN, KHET SUAN LUANG,
BANGKOK, 10250 THAILAND.

Location :	-	
Ambient Temperature :	(23.0 ± 3)	°C
Pressure :	(101.3 ± 3)	kPa
Relative Humidity :	(50.0 ± 20)	%

Received Date : 07 JANUARY 2025
Calibration Date : 21 - 23 JANUARY 2025
Date of Issue : 24 JANUARY 2025

REVIEW BY .....
APPROVED BY.....
NEXT CAL DATE.....21/ 01/ 2026.....

Calibrated by : Nathakorn Pisutpaisan

Approved by :

(Thanakul Petchurai)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

Cert. No. : ACL25072
Job No. : VC68AC0059
Pages : 2 of 8

Calibration Procedure : CP-AC-01

Calibration Method :

This equipment was calibrated by follow on IEC-61672-3 (2013) Standard for sound level meter (SLM).

The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.

For tests results of each items were made by observation of each Instruments display and also with SLM's display.

Condition of this result of calibration :

1. Reference Standard Instruments :

Instrument	Model	Serial No.	Cert. No.	Due Date
Waveform Generator	33210A	MY48017076	EF-0009-24	05-FEB-25
Waveform Generator	33511B	MY52302742	EF-0007-24	05-FEB-25
Digital Multimeter	33461A	MY53220104	EEL.BP 21/0267	13-FEB-25
Digital Multimeter	33461A	MY53220076	EEL.BP 20/0267	15-FEB-25
Digital Multimeter	34461A	MY60024273	EEL.BP 22/0267	15-FEB-25
Programmable Attenuator	MAT-1070	62100114	EF-0008-24	05-FEB-25
Condenser Microphone	4180	2977900	AA-1001-24	12-FEB-25
Measuring Amplifier	NA-42KAI	34560495	AA-3001-24	05-FEB-25

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.
3. This certificate is traceable to the international system of unit maintained at :
   - 3.1 National Institute of Metrology (Thailand).
   - 3.2 Thailand Institute of Scientific and Technological Research (TISTR).

Cert. No. : ACL25072
Job No. : VC68AC0059
Pages : 3 of 8

Summary of Measurement Result :

Parameter	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	0.2	N/A
2. Self-generated noise	0.2	N/A
3. Acoustical signal tests of frequency weightings		
125 Hz	0.3	0.6
1000 Hz	0.3	0.6
8000 Hz	0.3	0.7
4. Electrical signal tests of frequency weightings		
For 10 Hz to 4 kHz	0.3	0.6
For > 4 kHz to 10 kHz	0.3	0.7
For > 10 kHz to 20 kHz	0.3	1.0
5. Frequency and time weightings at 1 kHz	0.2	0.2
6. Long - term stability	0.1	0.1
7. Level linearity on the reference level range	0.2	0.3
8. Level linearity including the level range control	0.2	0.3
9. Tone burst response	0.2	0.3
10. Peak C sound level	0.2	0.35
11. Overload indication	0.2	0.25
12. High level stability	0.1	0.1

Cert. No. : **ACL25072**
Job No. : **VC68AC0059**
Page : **4 of 8**

Result of calibration :

1. Absolute sensitivity

Reference Acoustic Signal (dB)	Measured Value (dB)	Deviation (dB)	Acceptance Limit (dB)
93.9 (93.94)	93.9	0.0	±0.3

2. Self-generated noise

2.1 Normal test

Measured Value (dB)
16.0

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Weighting (dB)
A - weight	12.6
C - weight	17.7
Flat	22.6

3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
125	0.5	0.5	0.5	± 1.5
1000	0.1	0.1	0.1	± 1.0
8000	-1.2	-1.2	-1.2	±5.0

Cert. No. : ACL25072
Job No. : VC68AC0059
Pages : 5 of 8

4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	0.0	-0.1	-0.1	±2.0
125	-0.1	0.0	-0.1	±1.5
250	-0.1	0.0	-0.1	±1.5
500	0.0	0.0	-0.1	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.0	0.0	±2.0
4000	0.0	0.0	0.0	±3.0
8000	0.0	0.0	0.0	±5.0

5. Frequency and time weightings at 1 kHz

5.1 Frequency weightings at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.2
C - weight	94.0	94.0	0.0	± 0.2
Flat	94.0	94.0	0.0	± 0.2

5.2 Time weighting at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	94.0	94.0	0.0	± 0.1
Slow	94.0	94.0	0.0	± 0.1
Leq	94.0	94.0	0.0	± 0.1

6. Long - term stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.1	0.1	± 0.3

Cert. No. : ACL25072
Job No. : VC68AC0059
Pages : 6 of 8

7. Level linearity on the reference level range

Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
137.0	137.0	0.0	± 1.1
136.0	136.0	0.0	± 1.1
135.0	135.0	0.0	± 1.1
134.0	134.1	0.1	± 1.1
133.0	133.0	0.0	± 1.1
132.0	132.0	0.0	± 1.1
131.0	131.0	0.0	± 1.1
129.0	129.0	0.0	± 1.1
124.0	124.0	0.0	± 1.1
119.0	119.1	0.1	± 1.1
114.0	114.1	0.1	± 1.1
109.0	109.0	0.0	± 1.1
104.0	104.1	0.1	± 1.1
99.0	99.0	0.0	± 1.1
94.0	94.0	0.0	± 1.1
89.0	89.0	0.0	± 1.1
84.0	84.0	0.0	± 1.1
79.0	79.0	0.0	± 1.1
74.0	74.0	0.0	± 1.1
69.0	69.0	0.0	± 1.1
64.0	64.0	0.0	± 1.1
59.0	59.0	0.0	± 1.1
54.0	54.0	0.0	± 1.1
49.0	49.0	0.0	± 1.1
44.0	44.0	0.0	± 1.1
39.0	39.0	0.0	± 1.1
34.0	34.0	0.0	± 1.1
30.0	30.0	0.0	± 1.1
29.0	29.0	0.0	± 1.1
28.0	28.0	0.0	± 1.1
27.0	27.0	0.0	± 1.1
26.0	25.9	-0.1	± 1.1
25.0	24.9	-0.1	± 1.1

Cert. No. : ACL25072
Job No. : VC68AC0059
Pages : 7 of 8

8. Level linearity including the level range control

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
130	94.0	94.0	0.0	±1.1

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
130	29.0	29.0	0.0	±1.1

9. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Cycle	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	0.25	1	108.0	108.0	0.0	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.1	0.1	±1.0
Slow	2	8	108.0	108.1	0.1	1.5 ; -5.0
	200	800	127.6	127.7	0.1	±1.0
SEL	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.1	0.1	±1.0

10. Peak C sound level

Number of cycle in test signal	Anticipated Value (dB)	Measured Value, Lcpeak (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	130.0	130.0	0.0	±3.0
One	133.4	133.4	0.0	±3.0

Number of cycle in test signal	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	±2.0
Positive half cycle	135.4	135.1	-0.3	±2.0
Negative half cycle	135.4	135.1	-0.3	±2.0

11. Overload indication

Measured value (dB)		Deviated Value (dB)	Acceptance Limits (dB)
Positive one-half cycle	Negative one-half cycle		
89.5	89.5	0.0	±1.5

12. High level stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor $k = 2$ or any value following calculation,providing a lavel of confidence of approximately 95 %

End of Calibration Certificate

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7/139 MOO 13, SOI SUNTINAKORN 11 TAMBON BANG KAEO,
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAN
TEL: (66)0-2116-5860-1 FAX: (66)0-2116-7140

Certificate of Calibration

Customer

Name : ALS Laboratory Group Thailand Co., Ltd. **Certificate No :** 25-SLM-114

Address : 104 Soi Phatthanakan 40, Phatthanakan Road, Suan Luang, Bangkok 10250 **Request No :** Req-2025-0603

Unit Under Calibration Details

Measurement item :	Sound Level Meter	Microphone Class :	2
Manufacturer	RION	Microphone Model :	UC-52
Model	NL-42	Microphone S/N :	143841
Serial Number	01222723	Preamplifier Model :	NH-24
ID	RYG_FS0022	Preamplifier S/N :	22770
Resolution	0.1 dB	Instrument Status :	Used

Calibration Environment and Details

Temperature : 23 °C ± 2 °C

Humidity : 50 %RH ± 20 %RH

Barometric Pressure : 1013 hPa ± 10 hPa

Received Date : 6 March 2025

Calibrated Date : 19 March 2025

Calibration Procedure : In-house method CP-SLM-01 based on IEC 61672-3 : 2013 Electroacoustics - Sound level meters - Part 3: Periodic tests

Location of Calibration : Lab Acoustic

REVIEW BY ..... Narakorn P.

APPROVED BY .....

NEXT CAL DATE..... 19/03/26 .....

Reference Standard

Instrument	**Brand**	Model	SN.	Due calibration	Tracebility
Standard Microphone	Brüel & Kjær	4192	2294985	25 June 2025	NIMT
Audio Generator	Svantek	Svan401	131	15 October 2025	WK Electric

Note

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor k = 2, providing a level of confidence approximately 95 %.

Calibrated By :

Mr. Noppadon Luangart

Service Calibration Engineer

Approved By :

Mr. Pacit Mathavorn

Calibration Engineer Supervisor

Issue Date : 19 March 2025

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7/139 MOO 13, SOI SUNTINAKORN 11 TAMBON BANG KAEO,
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAN
TEL: (66)0-2116-5860-1 FAX: (66)0-2116-7140

Certificate No : 25-SLM-114

Request No : Req-2025-0603

1. Indication at the calibration check frequency

UUC Setting	Nominal	Before Adjust		After Adjust		UNCERTAINTY	Acceptance	Result
FAST / A / 30-130	Level	UUC	ERR	UUC	ERR		Limit	
Calibrator Setting	(dB)	(dB)	(dB)	(dB)	(dB)	(± dB)	(± dB)	
1000 Hz 94 dB	94.06	94.0	-0.06	94.1	+0.04	0.20	0.30	Pass

Note : Absolute sensitivity was established by the use of Sound Calibrator Brand RION, Model NC-75, SN.35002736

2. Self-generated noise, Microphone installed

UUC Setting	Measured	UNCERTAINTY
FAST / 30-130		
UUC Weighting	(dB)	(± dB)
A	15.4	0.10

3. Self-generated noise, Microphone replaced by the electrical input signal device

UUC Setting	Measured	UNCERTAINTY
FAST / 30-130		
UUC Weighting	(dB)	(± dB)
A	12.2	0.10
C	16.6	0.10
Z	20.4	0.10

4. Acoustic signal test of frequency weightings (Without Windscreen)

UUC Setting	Deviation from various Frequency Weighting Respone curve			UNCERTAINTY	Acceptance Limit	Result
FAST / 30-130	A	C	Z	(± dB)	(± dB)	
STD Setting	(dB)	(dB)	(dB)			
125 Hz	0.3	0.5	0.5	0.60	1.5	Pass
1000 Hz	0.0	0.0	0.0	0.60	1.0	Pass
4000 Hz	0.4	0.4	0.4	0.60	3.0	Pass
8000 Hz	-1.3	-1.3	-1.3	0.70	5.0	Pass1

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7/139 MOO 13, SOI SUNTINAKORN 11 TAMBON BANG KAEO,
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAN
TEL: (66)0-2116-5860-1 FAX: (66)0-2116-7140

Certificate No : 25-SLM-114

Request No : Req-2025-0603

5. Electrical signal test of frequency weightings, Weighting network respone with relative to 1 kHz

UUC Setting	Deviation from various Frequency			UNCERTAINTY	Acceptance	Result
FAST / 30-130	Weighting Respone curve				Limit	
STD Setting	A (dB)	C (dB)	Z (dB)	(± dB)	(± dB)	
63 Hz	-0.1	0.0	0.0	0.20	2.0	Pass
125 Hz	-0.1	0.0	0.0		1.5	Pass
250 Hz	0.0	0.0	0.0		1.5	Pass
500 Hz	0.0	0.1	0.0		1.5	Pass
1000 Hz	0.0	0.0	0.0		1.0	Pass
2000 Hz	0.0	0.1	0.0		2.0	Pass
4000 Hz	0.0	0.0	0.0		3.0	Pass
8000 Hz	0.1	0.1	0.0		5.0	Pass
16000 Hz	-1.3	-1.3	0.0		+5, -INF.	Pass

6. Frequency and time weightings at 1kHz

UUC Setting	STD	Measured		UNCERTAINTY	Acceptance	Result
FAST / 30-130	REF	UUC	ERR		Limit	
UUC Weighting	(dB)	(dB)	(dB)	(± dB)	(± dB)	
A	114.00	114.0	0.0	0.20	0.20	Pass
C	114.00	114.0	0.0		0.20	Pass
Z	114.00	114.0	0.0		0.20	Pass

UUC Setting	STD	Measured		UNCERTAINTY	Acceptance	Result
30-130 / A	REF	UUC	ERR		Limit	
UUC Time Respone	(dB)	(dB)	(dB)	(± dB)	(± dB)	
Fast	114.00	114.0	0.0	0.20	0.10	Pass1
Slow	114.00	114.0	0.0		0.10	Pass1
Leq	114.00	114.0	0.0		0.10	Pass1

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7/139 MOO 13, SOI SUNTINAKORN 11 TAMBON BANG KAEO,
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAN
TEL: (66)0-2116-5860-1 FAX: (66)0-2116-7140

Certificate No : 25-SLM-114

Request No : Req-2025-0603

7. Long Term Stability

UUC Setting	Measured	UNCERTAINTY	Acceptance Limit	Result
FAST / A / 30-130	UUC			
STD Setting	(dB)	(± dB)	(± dB)	
Initial	114.0			
Final	114.0			
Deviated	0.0	0.10	0.30	Pass

8. Level linearity on the reference level range

UUC Setting	Anticipated	Deviation		UNCERTAINTY	Acceptance	Result
FAST / A / 30-130	REF	UUC	ERR		Limit	
STD dB	(dB)	(dB)	(dB)	(± dB)	(± dB)	
138.00	138	137.9	-0.1	0.30	1.1	Pass
134.00	134	134.0	0.0		1.1	Pass
129.00	129	129.0	0.0		1.1	Pass
124.00	124	124.0	0.0		1.1	Pass
119.00	119	119.0	0.0		1.1	Pass
114.00	114	114.0	0.0		1.1	Pass
109.00	109	109.0	0.0		1.1	Pass
104.00	104	104.0	0.0		1.1	Pass
99.00	99	99.0	0.0		1.1	Pass
94.00	94	94.0	0.0		1.1	Pass
89.00	89	89.0	0.0		1.1	Pass
84.00	84	84.0	0.0		1.1	Pass
79.00	79	79.0	0.0		1.1	Pass
74.00	74	74.0	0.0		1.1	Pass
69.00	69	69.0	0.0		1.1	Pass
64.00	64	64.0	0.0		1.1	Pass
59.00	59	59.0	0.0		1.1	Pass
54.00	54	54.0	0.0		1.1	Pass
49.00	49	49.0	0.0		1.1	Pass
44.00	44	44.0	0.0		1.1	Pass
39.00	39	39.0	0.0		1.1	Pass
34.00	34	34.0	0.0		1.1	Pass
29.00	29	29.1	0.1		1.1	Pass
24.00	24	24.0	0.0		1.1	Pass

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7/139 MOO 13, SOI SUNTINAKORN 11 TAMBON BANG KAEO,
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAN
TEL: (66)0-2116-5860-1 FAX: (66)0-2116-7140

Certificate No : 25-SLM-114

Request No : Req-2025-0603

9. Level linearity including the level range control

UUC Setting	STD	Measured		UNCERTAINTY	Acceptance	Result
FAST / A	REF	UUC	ERR		Limit	
UUC Range	(dB)	(dB)	(dB)	(± dB)	(± dB)	
30-130	29.50	29.7	0.2	0.30	1.1	Pass
	114	114.0	0.0		1.1	Pass

10. Tone burst response

UUC Setting	STD	Anticipated	Measured		UNCERTAINTY	Acceptance	Result
A / 30-130	Toneburst	Ref	UUC	ERR		Limit	
UUC Time Respone	(ms)	(dB)	(dB)	(dB)	(± dB)	(± dB)	
Fast	200	126.0	126.1	+0.1	0.20	1.0	Pass
	2	109.0	109.0	0.0		+1.0, -2.5	Pass
	0.25	100.0	99.9	-0.1		+1.5, -5.0	Pass
Slow	200	119.6	119.6	0.0		1.0	Pass
	2	100.0	100.0	0.0		+1.0, -5.0	Pass
SEL	200	120.0	120.0	0.0		1.0	Pass
	2	100.0	100.0	0.0		+1.0, -2.5	Pass
	0.25	91.0	90.9	-0.1		+1.5, -5.0	Pass

11. Peak C Sound level

UUC Setting	Anticipated	Measured		UNCERTAINTY	Acceptance	Result
FAST / C / 55-141	REF	UUC	ERR		Limit	
STD Setting	(dB)	(dB)	(dB)	(± dB)	(± dB)	
Complete cycle	136.4	135.8	-0.60	0.20	3.0	Pass
Positive half cycle	135.4	135.2	-0.20		2.0	Pass
Negative half cycle	135.4	135.2	-0.20		2.0	Pass

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7/139 MOO 13, SOI SUNTINAKORN 11 TAMBON BANG KAEO,
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL: (66)0-2116-5860-1 FAX: (66)0-2116-7140

Certificate No : 25-SLM-114

Request No : Req-2025-0603

12. Overload indication

UUC Setting / STD Setting	Measured UUC (dB)	UNCERTAINTY (± dB)	Acceptance Limit (± dB)	Result
FAST / A / 30-130				
Positive one-half cycle	139.5			
Negative one-half cycle	139.4			
Deviated	0.1	0.20	1.5	Pass

13. High Level Stability

UUC Setting / STD Setting	Measured UUC (dB)	UNCERTAINTY (± dB)	Acceptance Limit (± dB)	Result
FAST / A / 30-130				
Initial	129.0			
Final	129.0			
Deviated	0.0	0.10	0.30	Pass

Note :

Function	Maximum-permitted Uncertainty of measurement
1. Indication at the calibration check frequency	Not applicable
2. Self-generated noise, Microphone installed	Not applicable
3. Self-generated noise, Microphone replaced by the electrical input signal device	Not applicable
4. Acoustic signal test of frequency weightings at 10 Hz to 4 kHz	0.60 dB
4. Acoustic signal test of frequency weightings at >4 kHz to 10 kHz	0.70 dB
5. Electrical signal test of frequency weightings, Weighting network respone with relative to 1 kHz	0.20 dB
6. Frequency and time weightings at 1kHz	0.20 dB
7. Long Term Stability	0.10 dB
8. Level linearity on the reference level range	0.30 dB
9. Level linearity including the level range control	0.30 dB
10. Tone burst response	0.30 dB
11. Peak C Sound level	0.35 dB
12. Overload indication	0.25 dB
13. High Level Stability	0.10 dB

- Acceptance limit and Maximum-permitted Uncertainty was IEC 61672-1:2013

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7/139 MOO 13, SOI SUNTINAKORN 11 TAMBON BANG KAEO,
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAN
TEL: (66)0-2116-5860-1 FAX: (66)0-2116-7140

Certificate No : 25-SLM-114

Request No : Req-2025-0603

Decision Rule for Statements of Conformity

The standard decision rule employed for the statements of conformity to each calibration result will be applied using ILAC-G8:09/2019; Guidelines on the Reporting of Compliance with Specification as following Fig. and statements

Pass = The measurement result plus the expanded uncertainty with a 95% coverage probability were within the limit.

Pass[1] = The measurement result was within the limit. However, a portion of the expanded uncertainty of measurement at 95% exceeds the limit.

Fail[1] = The measurement result was out of the limit. However, a portion of the expanded uncertainty of measurement at 95% is within the limit.

Fail = The measurement result plus the expanded uncertainty with a 95% coverage probability were outside the limit.

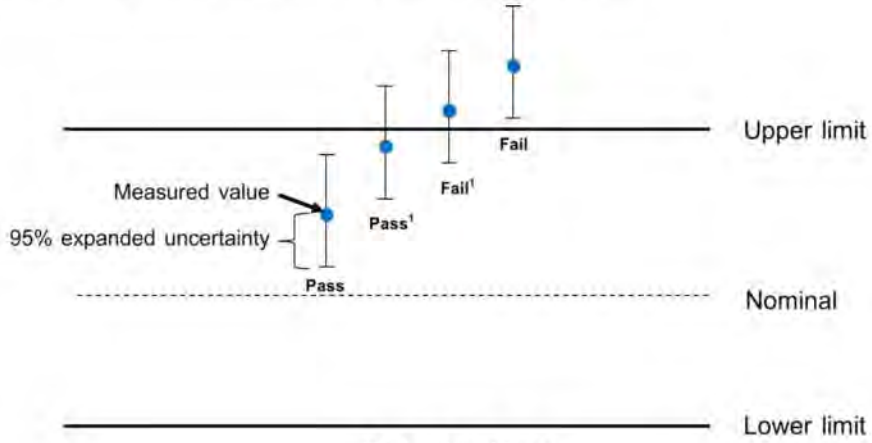

End of Certificate

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd

SITHIPORN ASSOCIATES CO., LTD.
CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand
Tel. +66 2433 8331 Email : calibration@sithiphorn.com

NSC-TISI-TIS 17025
CALIBRATION 0394

Calibration Certificate

Equipment :	SOUND LEVEL METER
Manufacturer :	RION
Model :	NL-42 / Microphone UC-52 / Preamplifier NH-24
Serial No.:	00296518 / 66239 / 34375
ID No.:	RYG_FS0431

Condition As Found : GOOD

Customer : ALS LABORATORY GROUP (THAILAND) CO., LTD.
104 PHATTHANAKAN 40, PHATTHANAKAN ROAD,
KHWAENG PHATTHANAKAN, KHET SUAN LUANG,
BANGKOK, 10250 THAILAND.

Location :	-	
Ambient Temperature :	(23.0 ± 3)	°C
Pressure :	(101.3 ± 3)	kPa
Relative Humidity :	(50.0 ± 20)	%

Received Date : 14 JANUARY 2025
Calibration Date : 27-29 JANUARY 2025
Date of Issue : 30 JANUARY 2025

REVIEW BY .....
APPROVED BY.....
NEXT CAL DATE.....26/ 01/ 2026.....

Calibrated by : Nathakorn Pisutpaisan

Approved by :

(Thanakul Petchurai)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

Cert. No. : ACL25105
Job No. : VC68AC0064
Pages : 2 of 8

Calibration Procedure : CP-AC-01

Calibration Method :

This equipment was calibrated by follow on IEC-61672-3 (2013) Standard for sound level meter (SLM).
The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.
For tests results of each items were made by observation of each Instruments display and also with SLM's display.

Condition of this result of calibration :

1. Reference Standard Instruments :

Instrument	Model	Serial No.	Cert. No.	Due Date
Waveform Generator	33210A	MY48017076	EF-0009-24	05-FEB-25
Waveform Generator	33511B	MY52302742	EF-0007-24	05-FEB-25
Digital Multimeter	33461A	MY53220104	EEL.BP 21/0267	13-FEB-25
Digital Multimeter	33461A	MY53220076	EEL.BP 20/0267	15-FEB-25
Digital Multimeter	34461A	MY60024273	EEL.BP 22/0267	15-FEB-25
Programmable Attenuator	MAT-1070	62100114	EF-0008-24	05-FEB-25
Condenser Microphone	4180	2977900	AA-1001-24	12-FEB-25
Measuring Amplifier	NA-42KAI	34560495	AA-3001-24	05-FEB-25

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.
3. This certificate is traceable to the international system of unit maintained at :
   - 3.1 National Institute of Metrology (Thailand).
   - 3.2 Thailand Institute of Scientific and Technological Research (TISTR).

Cert. No. : ACL25105
Job No. : VC68AC0064
Pages : 3 of 8

Summary of Measurement Result :

Parameter	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	0.2	N/A
2. Self-generated noise	0.2	N/A
3. Acoustical signal tests of frequency weightings		
125 Hz	0.3	0.6
1000 Hz	0.3	0.6
8000 Hz	0.3	0.7
4. Electrical signal tests of frequency weightings		
For 10 Hz to 4 kHz	0.3	0.6
For > 4 kHz to 10 kHz	0.3	0.7
For > 10 kHz to 20 kHz	0.3	1.0
5. Frequency and time weightings at 1 kHz	0.2	0.2
6. Long - term stability	0.1	0.1
7. Level linearity on the reference level range	0.2	0.3
8. Level linearity including the level range control	0.2	0.3
9. Tone burst response	0.2	0.3
10. Peak C sound level	0.2	0.35
11. Overload indication	0.2	0.25
12. High level stability	0.1	0.1

Cert. No. : ACL25105
Job No. : VC68AC0064
Page : 4 of 8

Result of calibration :

1. Absolute sensitivity

Reference Acoustic Signal (dB)	Measured Value (dB)	Deviation (dB)	Acceptance Limit (dB)
93.9 (93.94)	93.9	0.0	±0.3

2. Self-generated noise

2.1 Normal test

Measured Value (dB)
22.0

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Weighting (dB)
A - weight	14.2
C - weight	20.1
Flat	25.8

3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
125	0.3	0.3	0.3	± 1.5
1000	0.2	0.2	0.2	± 1.0
8000	1.1	1.1	1.1	±5.0

Cert. No. : ACL25105
Job No. : VC68AC0064
Pages : 5 of 8

4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	0.0	-0.1	-0.1	±2.0
125	0.0	0.0	0.0	±1.5
250	0.0	0.0	0.0	±1.5
500	0.0	0.0	0.0	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.0	0.0	±2.0
4000	0.0	0.0	0.0	±3.0
8000	0.0	0.1	0.1	±5.0

5. Frequency and time weightings at 1 kHz

5.1 Frequency weightings at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.2
C - weight	94.0	94.0	0.0	± 0.2
Flat	94.0	94.0	0.0	± 0.2

5.2 Time weighting at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	94.0	94.0	0.0	± 0.1
Slow	94.0	94.0	0.0	± 0.1
Leq	94.0	94.0	0.0	± 0.1

6. Long - term stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.3

Cert. No. : ACL25105
Job No. : VC68AC0064
Pages : 6 of 8

7. Level linearity on the reference level range

Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
137.0	137.0	0.0	± 1.1
136.0	136.0	0.0	± 1.1
135.0	135.0	0.0	± 1.1
134.0	134.0	0.0	± 1.1
133.0	133.0	0.0	± 1.1
132.0	132.0	0.0	± 1.1
131.0	131.0	0.0	± 1.1
129.0	129.0	0.0	± 1.1
124.0	124.0	0.0	± 1.1
119.0	119.0	0.0	± 1.1
114.0	114.0	0.0	± 1.1
109.0	109.0	0.0	± 1.1
104.0	104.0	0.0	± 1.1
99.0	99.0	0.0	± 1.1
94.0	94.0	0.0	± 1.1
89.0	89.1	0.1	± 1.1
84.0	84.1	0.1	± 1.1
79.0	79.0	0.0	± 1.1
74.0	74.1	0.1	± 1.1
69.0	69.1	0.1	± 1.1
64.0	64.0	0.0	± 1.1
59.0	59.1	0.1	± 1.1
54.0	54.0	0.0	± 1.1
49.0	49.0	0.0	± 1.1
44.0	44.0	0.0	± 1.1
39.0	39.0	0.0	± 1.1
34.0	34.0	0.0	± 1.1
30.0	30.0	0.0	± 1.1
29.0	29.0	0.0	± 1.1
28.0	28.0	0.0	± 1.1
27.0	26.9	-0.1	± 1.1
26.0	25.9	-0.1	± 1.1
25.0	25.0	0.0	± 1.1

Cert. No. : ACL25105
Job No. : VC68AC0064
Pages : 7 of 8

8. Level linearity including the level range control

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
130	94.0	94.0	0.0	±1.1

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
130	29.0	28.9	-0.1	±1.1

9. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Cycle	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.0	0.0	±1.0
Slow	2	8	108.0	108.0	0.0	1.5 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
SEL	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.1	0.1	±1.0

10. Peak C sound level

Number of cycle in test signal	Anticipated Value (dB)	Measured Value, Lcpeak (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	130.0	130.0	0.0	±3.0
One	133.4	133.3	-0.1	±3.0

Number of cycle in test signal	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	±2.0
Positive half cycle	135.4	135.2	-0.2	±2.0
Negative half cycle	135.4	135.2	-0.2	±2.0

11. Overload indication

Measured value (dB)		Deviated Value (dB)	Acceptance Limits (dB)
Positive one-half cycle	Negative one-half cycle		
89.6	89.5	-0.1	±1.5

12. High level stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor $k = 2$ or any value following calculation,providing a lavel of confidence of approximately 95 %

End of Calibration Certificate

TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL.0-2717-3000-29 FAX.0-2719-9484

NSC-TISI-TIS17025
CALIBRATION 0008

Certificate of Calibration

Cert.No.: 25CH847
Page.: 1 of 3

Equipment :	pH Meter
Manufacturer :	Mettler Toledo
Model :	SevenCompact S220
Serial No. :	C104059460
ID No. :	RYG_EN0183
Condition As-Received:	Used Item
Received Date :	17 July 2025
Calibration Date :	18 July 2025
Reference :	2507-0561DSC-3
Submitted by :	ALS Laboratory Group (Thailand) Co.,Ltd. Rayong Branch 616/10 Moo 5, T.Maenam Khu, A.Pluakdaeng, Rayong 21140, Thailand
Ambient Temperature :	(25 ± 2.5) °C
Relative Humidity :	(50 ± 15) %
Calibration Procedure :	In - house method : - CP-CH5 by direct measurement with DC voltage standard and direct measurement with certified reference material (CRM) - CP-CH8 by comparison with temperature standard

REVIEW BY ..... PhotchanaS.

APPROVED BY .....

NEXT CAL DATE..... 18/01/27 .....

Calibrated by : Walalak Sirithean

Approved by : Saithip

Approved Signatory

( ) Chakrit Waewwanjua
( ) Ponpan Paipim
(✓) Saithip Meangmai

Issue Date : 21 July 2025

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

Condition of this calibration result

1. Reference Standard Instrument

Instrument	Serial No.	ID No.	Cert. No.	Due Date
1) Document Process Calibrator	54030049	130RC116	24E2759	25 Aug 2025
2) Ref. Standard Thermometer	3240076	60RC033	25I394	01 Apr 2026

- This measurement result is traceable to SI throught Technology Promotion Association (Thailand - Japan)

2. Certified Reference Materials : The measurement results are traceable to SI through CPA chem Ltd., ANSI-ASQ National Accreditation Board, Accredited No. AR-1835

Buffer Solution	Manufacturer	Lot No.	Exp. date
pH 4.007	CPA chem	1066665	18 Jan 2027
pH 6.965	CPA chem	1066667	18 Jan 2026
pH 10.010	CPA chem	1114385	08 June 2026

3. This certificate is valid only to the item calibrated on date and place of calibration.

Calibration Results

Function : mV Measurement

Performing standard curve by Document Process Calibrator at pH (4,7,10)

Unit Under Calibration	Nominal Value	Standard Voltage Input	Actual Reading		Uncertainty of Measurement (±mV)	Coverage factor *k*
	pH	mV	mV	pH		
pH Meter	4.000	177.48	177.3	4.000	0.058	2.00
S/N.: C104059460	7.000	0.00	-0.2	7.000	0.058	2.00
	10.000	-177.48	-177.6	10.000	0.058	2.00

Calibration Results

Function : pH Measurement

Performing three buffers standard curve by using buffer nominal pH (4,7,10)

Unit Under Calibration	Standard pH Buffer Solution	Actual pH Reading	Actual mV Reading (mV)	Uncertainty of pH Measurement (±)	Coverage factor *k*
pH Electrode	4.007	4.008	184.6	0.0044	2.00
S/N.: 5240606	6.965	6.966	10.2	0.0084	2.00
	10.010	10.009	-164.9	0.0065	2.00

Function : Temperature Measurement

(*) Without adjustment

This equipment was connected with Temperature Probe;

- Model : InLabExpert Pro-ISM
- Serial No. : 5240606

Dimension of probe

- Length : 120 mm.
- Diameter : 12 mm.
- Immersion Depth : 100 mm.

Calibration Point (°C)	Standard Temperature (°C)	UUC* Reading (°C)	Error (°C)	Uncertainty of measurement (± °C)	Coverage factor *k*
25.0	25.001	25.0	-0.001	0.13	2.00

Remark - UUC* = Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG, BANGKOK 10250
TEL. 0-2717-3000-24 FAX. 0-2719-9484

NSC-TISI-TIS17025
CALIBRATION 0008

Certificate of Calibration

Certificate No. : 25E2372

Equipment : pH Meter
Manufacturer: Mettler Toledo
Model : SevenCompact S220
Serial No.: C104059460
ID No.: RYG_EN0183
Condition As-Received: Used Item
Received Date: 17 July 2025
Calibration Date: 22 July 2025

This certificate may not be reproduced other than in full,
except with the prior written approval of the head of
Corporate Services 3: Equipment Calibration and Testing Services.

Reference: 2507-0561DSC
Ambient Temperature: (23 ± 2) °C
Relative Humidity: (50 ± 10) %

Submitted by: ALS Laboratory Group (Thailand) Co.,Ltd. Rayong Branch

616/10 Moo 5, T.Maenam Khu, A.Pluakdaeng,
Rayong 21140, Thailand

Procedure used: Calibration were conducted using calibration procedure No. CP-E17 according to EURAMET cg-15.

Condition of this result of calibration

1.Reference standards instruments :

Instrument	Model	Serial No.	Certificate No.	Due Date
1) Multi-Product Calibrator	5500A	6315011	25E1627	19 May 2026

2.This result of calibration was made on requested at the point specified by customer.

3.The certificate is valid only to the item calibrated on date and place of calibration.

4.This measurement result is traceable to the International System of Unit maintained through:-

-Technology Promotion Association (Thailand-Japan), NSC-ONSC Accredited No. Calibration 0008

Calibrated by : Napachanok Prasomsoosiri
Issue Date : 23 July 2025

Approved Signatory : _____

[ ] Phalinee Prabpaipal
[ ] Nuntawat Khamchai
[✓] Pongsagorn Boonyaporn

Result of calibration :- (*) Without adjustment ( ) After adjustment

Function: DC voltage measurement **Range:** 2000 mV

Standard Value (mV)	UUC* Reading (mV)	Error (mV)	Uncertainty (± µV)
-200.0000	-200.0	0.0	68
-150.0000	-150.0	0.0	65
-100.0000	-100.0	0.0	63
-50.0000	-50.0	0.0	61
0.0000	0.0	0.0	58
50.0000	49.9	-0.1	61
100.0000	99.9	-0.1	63
150.0000	149.9	-0.1	65
200.0000	199.9	-0.1	68

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k = 2, providing a level of confidence of approximately 95 %

UUC* = Unit Under Calibration.

-o0o-

TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL.0-2717-3000-29 FAX.0-2719-9484

NSC-TISI-TIS17025
CALIBRATION 0008

Certificate of Calibration

Cert. No.: 25LM10

Equipment :	DO Meter with Sensor
Manufacturer :	YSI
Model :	5000-115V
Serial No. :	15E102796
ID No. :	RYG_EN0032
Submitted by :	ALS Laboratory Group (Thailand) Co.,Ltd. (Rayong Branch) 616/10 Moo 5 T. Maenam Khu, A. Pluakdaeng, Rayong 21140 Thailand
Location :	TPA On Site Calibration Laboratory
Received Order :	17 January 2025
Calibrated Date :	20 January 2025
Ambient Temperature :	(26 ± 10) °C
Relative Humidity :	(50 ± 30) %
AC Line Voltage :	(220 ± 22) V
Calibrated by :	Warakorn Lerngagtrakul
Approved by :	Approved Signatory

REVIEW BY Photchana S.
APPROVED BY D. Khunou.
NEXT CAL DATE 20/07/26

( ) Chakrit Waewwanjua
(✓) Suwit Imjai
( ) Kunchit Promprat

Issue Date : 23 January 2025

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

Equipment : DO Meter with Sensor **Cert. No.:** 25LM10

Condition As-Received : Used Item

Reference : 2501-0600DSC-2

Procedure Used :-

Calibration were conducted using in-house calibration procedure CP-OT01 according to comparison with Industrial Platinum Resistance Thermometer (IPRT) into Temperature Bath.

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

Instrument	Serial No.	Cert. No.	Traceable	Due Date
1) Digital Thermometer	2188080	24I1022	TPA	17 Sep 2025

2. This certificate is valid only to the item calibrated on date and place of calibration.
3. This certification is traceable to the International System of Unit.

Remark : TPA : Technology Promotion Association (Thailand - Japan)

Result of Calibration :- (*) Without Adjustment

Function : Temperature measurement.

This instrument was connected with temperature sensor, S/N.: 15E100464

Calibration Point (°C)	Immersion Depth (mm)	Standard Temperature (°C)	UUC* Reading (°C)	Error (°C)	Uncertainty (± °C)	Coverage Factor *k*
20.00	60	20.002	19.81	-0.192	0.15	2.00

UUC* : Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor ***k***, providing a level of confidence of approximately 95 %.

-o0o-

TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3 : EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000 FAX. 0-2719-9484

Certificate of Testing

Equipment :	DO Meter
Manufacturer :	YSI
Model :	5000-115V
Serial No. :	15E102796
ID No. :	RYG_EN0032
Received Date :	17 January 2025
Test Date :	20 January 2025
Reference :	2501-0600DSC-1
Submitted by :	ALS Laboratory Group (Thailand) Co.,Ltd. (Rayong Branch) 616/10 Moo 5, T.Maenam Khu, A.Pluakdaeng, Rayong 21140, Thailand
Laboratory Condition :	Temperature (25 ± 5) °C Humidity (50 ± 20) %
Test Procedure :	In - house method : CP-CH9 by Comparison Technique with Azide Modification Method
Tested by :	Walalak Sirithean
Approved by :	Saithip Approved Signatory

( ) Pornthippa Tameyakul
( ) Ponpan Paipim
(✓) Saithip Meangmai

Issue Date : 21 January 2025

Condition of this result of calibration

1. Reference Standard Instruments :
   This certification is traceable to the International System of Unit through the reference standards laboratory of Industrial Calibration Center, Technology Promotion Association (Thailand-Japan).

Instruments	Serial No.	ID No.	Certificate No.	Due Date
1. Burette	-	130BU10	23CG1172	22 Mar 2025
2. Balance	14233821	110RC001	24MM131	04 July 2025

2. Standard Material :-

Material	Manufacturer	Lot.No.	Assay
Sodium Thiosulfate 5-Hydrate AR	KEMAUS	2203162447	99.6%

Result : **Dissolved Oxygen Meter Adjustment With Air 100 %**
Dissolved Oxygen Probe No.: 15E100464

Titration Method (Azide Modification Method) (mg/L)	**DO Meter Reading** (mg/L)	**Standard Deviation** (mg/L)
8.20	8.20	0.0084

This report was certified only for the instrument we tested.It is allowable to use for study Intend to use for advertising and referral purpose is prohibited.This report may not be reproduced other in full, without written approval of the laboratory

-o0o-

TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL.0-2717-3000-29 FAX.0-2719-9484

NSC-TISI-TIS17025
CALIBRATION 0008

Certificate of Calibration

Cert. No.: 24TM1663
Page : 1 of 3

Equipment :	Low Temp. Incubator
Manufacturer :	Memmert
Model :	IPP750
Serial No. :	V818.0084
ID No. :	RYG_EN0154
Submitted by :	ALS Laboratory Group (Thailand) Co.,Ltd. Rayong Branch 616/10 Moo 5, T.Maenam Khu, A.Pluakdaeng, Rayong 21140, Thailand
Location :	BOD Room
Received Order :	01 November 2024
Calibration Date :	01 November 2024
Ambient Temperature :	(26 ± 10) °C
Relative Humidity :	(50 ± 30) %
AC Line Voltage :	(220 ± 22) V

REVIEW BY ..... Thanitak.

APPROVED BY..... D.Khunou.

NEXT CAL DATE..... 01/05/26

Calibrated by : Krisda Malee

Approved by : Kunchit

Approved Signatory

( ) Ponpan Paipim
( ) Suwit Imjai
(✓) Kunchit Promprat

Issue Date : 07 November 2024

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

Equipment : Low Temp. Incubator **Cert. No.:** 24TM1663

Condition As-Received : Used Item **Page :** 2 of 3

Reference : 2411-0002OC-1

Procedure Used :-

Calibration were conducted using calibration procedure CP-OT02 based on TLAS G-20 according to direct measurement method with Data Acquisition which connected with Resistance Temperature Detector (RTD).

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

Instrument	Serial No.	Cert. No.	Traceable	Due Date
1) Data Acquisition	MY44073381	24LM73	TPA	18 May 2025

2. This certificate is valid only to the item calibrated on date and place of calibration.
3. This certification is traceable to the International System of Unit.

Remark : TPA : Technology Promotion Association (Thailand - Japan)

Result of Calibration :- (*) Without Adjustment

Function of UUC* : Temperature Source

Fresh air setting : Close

Environment during calibration		
	Beginning	Finished
Temp. (°C)	24	25
REL.Humid. (%)	55	53
AC Supply (Volt)	220	221

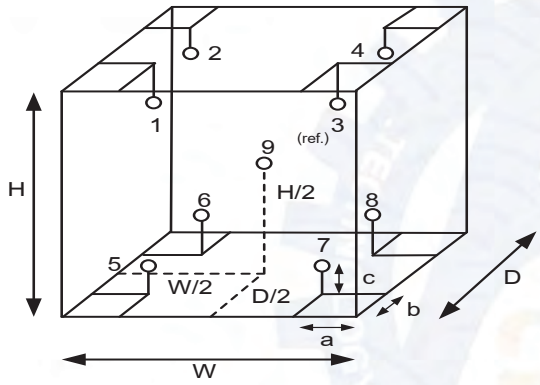

Position :	Ref. Std. ID No.:
1	1RTD-2/1
2	1RTD-2/2
3	22-01RTD-03
4	1RTD-2/4
5	1RTD-2/5
6	1RTD-2/6
7	23-01RTD-07
8	1RTD-2/8
9 (ref.)	23-01RTD-09

Probe Installation Details :

a =	10	cm
b =	10	cm
c =	10	cm

Dimension of Chamber :

D =	0.60	m
W =	1.0	m
H =	1.2	m
Capacity =	0.72	m^3

Equipment : Low Temp. Incubator
Condition As-Received : Used Item
Reference : 2411-0002OC-1
Result of Calibration :- (*) Without Adjustment
Function of UUC* : Temperature Source
Fresh air setting : Close

Cert. No.: 24TM1663

Calibration Point (°C)	UUC* Setting (°C)	UUC* Reading (°C)	Temperature stability (± °C)	Temperature uniformity (°C)	Overall Variation (°C)	Coverage Factor *k*
20.0	20.0	20.0	0.026	0.26	0.53	2

Calibration Point (°C)	Measured Temperature (°C) Position									Uncertainty (±°C)
	1	2	3	4	5	6	7	8	9 (ref.)	
20.0	20.071	19.915	20.273	20.179	19.977	19.782	20.056	20.026	20.033	0.30

Average* : The average of 30 values in each position.
Temperature stability : One-half of the greatest maximum difference of measured temperature at any one sensor.
Temperature uniformity : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.
Overall Variation : The Difference of the maximum and minimum measured temperatures throughout observation.
UUC* : Unit Under Calibration
Note : The reported uncertainty of measurement was included stability and excluded uniformity .

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor ***k***, providing a level of confidence of approximately 95 %.

-o0o-

TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL.0-2717-3000-29 FAX.0-2719-9484

NSC-TISI-TIS17025
CALIBRATION 0008

Certificate of Calibration

Cert.No.: 24CG3711

Equipment :	Burette
Capacity :	50 mL
Serial No. :	-
ID. No. :	RYG_EN0216
Manufacturer :	Witeg
Made in :	Germany
Submitted by :	ALS Laboratory Group (Thailand) Co.,Ltd. Rayong Branch 616/10 Moo 5, T.Maenam Khu, A.Pluakdaeng Rayong 21140, Thailand
Ambient Temperature :	(20 ± 2.5) °C
Relative Humidity :	(50 ± 10) %
Barometric Pressure :	756 mmHg
Calibration Procedure :	ASTM E 542 - 01
Calibrated by :	Sa-ngeunkam Wongsa
Approved by :	Approved Signatory

REVIEW BY ..... Thanitak.
APPROVED BY.....
NEXT CAL DATE..... 24/09/25

(✓) Srisuda Khamtha
( ) Ponpan Paipim
( ) Unnopphol Harachai

Issue Date : 24 September 2024

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

Equipment : Burette
Received Date : 19 September 2024
Condition As-Received : Used Item
Calibration Date : 24 September 2024
Reference : 2409-0756DSC-3

Cert.No.: 24CG3711

Condition of this result of calibration

1. Reference Standard Instruments :

Instruments	Model	Serial No.	ID. No.	Certificate No.	Traceability	Due date
1) Balance	XP205	B134206712	140RC007	24MM316	TPA	15 July 2025
2) Data Logger	HL-20D	20683159	140EC012	23H2174	TPA	10 Oct 2024
3) Thermometer	-	1594592	140EC010	24I175	TPA	20 Feb 2025

This certification is traceable to SI Unit

2. The certificate is valid only to the item calibrated on date and place of calibration.
3. True value is converted to true volume at the standard temperature of 20 $^{\circ}$C

Calibration result :

Nominal capacity (mL)	Reading (mL)	Uncertainty (± mL)	*k* Factor
10	10.0259	0.0082	2.00
20	20.0214	0.0085	2.00
30	30.0006	0.0089	2.00
40	40.0003	0.0094	2.00
50	49.9988	0.011	2.00

Remark mL = cm^3

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k* , providing a level of confidence of approximately 95 %.

-o0o-

TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL.0-2717-3000-29 FAX.0-2719-9484

NSC-TISI-TIS17025
CALIBRATION 0008

Certificate of Calibration

Cert.No.: 25CG3668

Equipment :	Burette
Capacity :	50 mL
Serial No. :	-
ID. No. :	RYG_EN0216
Manufacturer :	Witeg
Made in :	Germany
Submitted by :	ALS Laboratory Group (Thailand) Co.,Ltd. Rayong Branch 616/10 Moo 5 T.MaenamKoo, A.Pluakdaeng Rayong 21140, Thailand
Ambient Temperature :	(20 ± 2.5) °C
Relative Humidity :	(50 ± 10) %
Barometric Pressure :	753 mmHg
Calibration Procedure :	ASTM E 542 - 01
Calibrated by :	Srisuda Khamtha
Approved by :	Approved Signatory

REVIEW BY ..... ThanitaK.

APPROVED BY..... D.Thanon.

NEXT CAL DATE..... 18/09/26

( ) Ponpan Paipim
(✓) Chakrit Waewwanjua

Issue Date : 19 September 2025

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

Equipment : Burette
Received Date : 16 September 2025
Condition As-Received : Used Item
Calibration Date : 18 September 2025
Reference : 2509-0564DSC-3

Cert.No.: 25CG3668

Condition of this result of calibration

1. Reference Standard Instruments :

Instruments	Model	Serial No.	ID. No.	Certificate No.	Traceability	Due date
1) Balance	XP205	B134206712	140RC007	25MM296	TPA	16 July 2026
2) Humidity/Baro/Temp	MHB-382SD	AM.42259	140EC016	25H1616	TPA	14 Aug 2026
3) Digital Thermometer	HH376	230806555	140EC013	25I1740	TPA	17 Jan 2026

This measurement result is traceable to SI Unit

2. The certificate is valid only to the item calibrated on date and place of calibration.
3. True value is converted to true volume at the standard temperature of 20 $^{\circ}$C

Calibration result :

Nominal capacity (mL)	Reading (mL)	Uncertainty (± mL)	*k* Factor
10	10.0264	0.0082	2.00
25	25.0141	0.0087	2.00
50	49.9952	0.010	2.00

Remark mL = cm^3

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k* , providing a level of confidence of approximately 95 %.

-o0o-

Accredited by

NSC-TISI-TIS 17025
Calibration 0426

Calibration certificate

Calibration Certificate No. 25BKL0002

Object	Electronic non-automatic weighing instrument
Manufacturer	Sartorius
Type	MCE224S-2S00-U
Serial | QM Ident. no.	38101399 | RYG_EN0163
Customer	ALS Laboratory Group (Thailand) Co.,Ltd. (Rayong Branch) 616/10 Moo 5 T.Maenam Khu, A.Pluak Daeng, Rayong 21140, Thailand.
Order no.	2230
Number of pages	4
Date of calibration	20 Feb 2025

This calibration certificate documents the traceability to national standards.

Uncertainties of measurements are taken into account when only statements of compliance are made.

This certificate was prepared by Sartorius Corporation in accordance to the current ISO/IEC 17025:2017 standard and Sartorius Work Instruction (Method) SOP WI 08.

This certificate relate and apply this equipment only.

REVIEW BY ..... ThanitaK.

APPROVED BY..... D.Chumon.

NEXT CAL DATE..... 20/02/26

This calibration certificate may not be reproduced other than in full except with the permission of NSC-TISI-TIS-17025 and the issuing laboratory. Calibration certificates without signature are not valid.

The user is obliged to have the object recalibrated at appropriate intervals.

Date	Approval of the Calibration Certificate	Person in charge
06 Mar 2025	Mr. Chonchai Inthana	Kachen Lalee

Calibration object

Single range instrument

Model	MCE224S-2S00-U
Serial Number	38101399
QM Ident. no | Inventory no.	RYG_EN0163 | ---

Maximum capacity (Max. load)	220.0000 g
Measured range	220.0000 g
Scale interval	0.0001 g

Place of calibration

Address	According to page 1
Department | Cost center	Laboratory Department. | ---
Building | Floor	--- | 1st Floor.
Room	Balance Room.
Maximum temperature variation at place of calibration	5 K

Calibration procedure

EURAMET cg-18, V4.0 - Guidelines on the Calibration of Non-Automatic Weighing Instruments

Test equipment

Test equipment type	Test equipment ID	Valid until
Thermometer	MHB-382SD s/nB011342 Traceable to SI unit through DKSH	21 Aug 2025
Test weight set OIML R111 E2	Certificate No.M2308197S ,E2(Traceable to SI unit through TCS)	23 Aug 2025

Adjustment Status

The measuring device was internally adjusted before the calibration.

Environmental and measuring conditions

Date of calibration	20 Feb 2025
Temperature at place of calibration | Temp. diff. $T_{weights}$ - T_{place}	24.4 °C | 0.6 K
Measuring conditions	The installation site is suitable. The device was levelled. Balance was loaded up to Max before test.
Comments	Humidity 58.0 %RH.

Measurement results | Measurement uncertainties

Repeatability

Test load (nominal): 10 g | 200 g		
	10 g	**200 g**
1	10.0000 g	200.0000 g
2	10.0000 g	200.0000 g
3	10.0000 g	200.0001 g
4	9.9999 g	200.0000 g
5	9.9999 g	200.0000 g
6	10.0000 g	200.0001 g
7	10.0000 g	200.0000 g
8	10.0000 g	200.0000 g
9	9.9999 g	200.0001 g
10	10.0000 g	200.0000 g
	s = 0.00005 g	s = 0.00005 g

Eccentricity

Test load (nominal):	**100 g**
Center	100.0000 g
Front left	100.0000 g
Back left	100.0000 g
Back right	100.0000 g
Front right	99.9999 g
Maximum deviation from centric loading indication $\lvert\Delta I_{ecc}\rvert_{max}$ = 0.0001 g	

Error of indication

Testload ***L***	**Indication** ***I***	**Error** ***E***	**Expansion factor** ***k***	**Uncertainty** ***U(E)***	**Uncertainty relative** $U_{rel}(E)$
0.0100 g	0.0100 g	0.0000 g	2.00	0.00013 g	1.3 %
0.1000 g	0.1000 g	0.0000 g	2.00	0.00013 g	0.13 %
0.5000 g	0.5000 g	0.0000 g	2.00	0.00013 g	0.026 %
1.0000 g	1.0000 g	0.0000 g	2.00	0.00013 g	0.013 %
5.0000 g	5.0000 g	0.0000 g	2.00	0.00013 g	0.0026 %
10.0000 g	9.9999 g	-0.0001 g	2.00	0.00013 g	0.0013 %
20.0000 g	20.0000 g	0.0000 g	2.00	0.00014 g	0.00068 %
50.0000 g	50.0001 g	0.0001 g	2.00	0.00015 g	0.00029 %
100.0000 g	100.0000 g	0.0000 g	2.00	0.00018 g	0.00018 %
200.0000 g	200.0000 g	0.0000 g	2.00	0.00028 g	0.00014 %
220.0000 g	220.0000 g	0.0000 g	2.00	0.00032 g	0.00015 %
Maximum error of indication		$\lvert E\rvert_{max}$ = 0.0001 g			

$U_{rel}(E)$ is the quotient of $U(E)$ and test load L. The uncertainty of measurement $U(E)$ is valid only if error E is considered. You will find reference notes on the uncertainty of measurement in use under: Appendix to the calibration certificate | Interpretation of measurement results.
Reference note: The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the documented Expansion factor, determined in accordance with the European Calibration Guideline EURAMET cg-18, V4.0. There is a 95 % probability that the value of the measurand will be in the assigned value range.

End of calibration certificate

Uncertainty of measurement in use

Device adjusted before measurement	Yes
Temperature deviation considered	1.5 K (isoCAL active)
Temperature coefficient considered	$1 \cdot 10^{-6}$/K
Uncertainty of the weighing result $U_{gl}(W)$	**$U_{gl}(W) = 0.00013\ g + 1.16 \cdot 10^{-5} \cdot R$**

Reference note: The current uncertainty of measurement is calculated by entering of the reading *R* into this formula. In relation to this, there is no need for a correction of the indication error. The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied with an Expansion factor of 2, determined in accordance with the European Calibration Guideline EURAMET cg-18, V4.0. There is a 95 % probability that the value of the measurand will be in the assigned value range.

Indication in % from max load	Net indication *R*	Uncertainty $U_{gl}(W)$	Uncertainty relative $U_{gl}(W)_{rel}$
1 %	2.2000 g	0.00016 g	0.0071 %
25 %	55.0000 g	0.00077 g	0.0014 %
50 %	110.0000 g	0.0014 g	0.0013 %
75 %	165.0000 g	0.0020 g	0.0012 %
100 %	220.0000 g	0.0027 g	0.0012 %

Graphic realization of the relative uncertainty of measurement | process accuracy

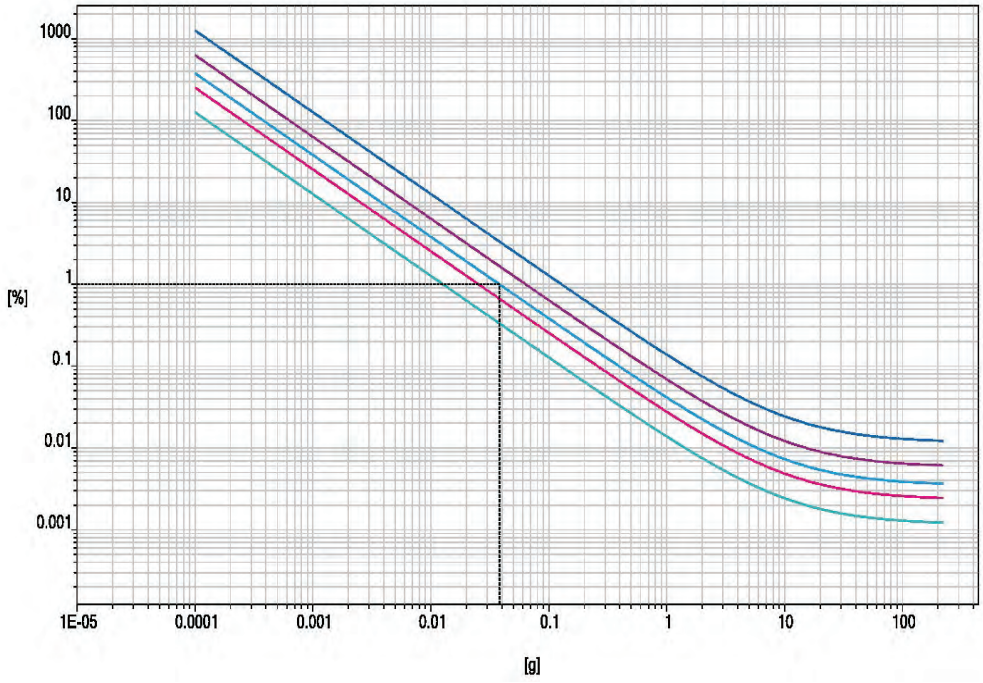

Safety factor
10
5
3
2
1

Displayed example

Process accuracy	1.00 %
Safety factor	3
Minimum sample weight	0.0381 g

Metrology Center
SCI ECO Services Company Limited
51 Moo 8, Tubkwang, Kaeng Khoi, Saraburi, Thailand 18260
Bangkok Tel : +668 9205 6851 , +669 81924 0059
Saraburi Tel : +669 8247 2360
Website : www.scieco.co.th E-Mail : calibrate@scg.co.th

NSC-TISI-TIS 17025
CALIBRATION 0244

Certificate No. T251530

Certificate of Calibration

Equipment	:	**Chamber (Oven)**
Manufacturer	:	**MEMMERT**
Model	:	**UF 110**
Serial No.	:	**B416.2420**
Customer Code	:	**RYG_EN0012**
ID No.	:	**T6444A5**
Customer	:	**ALS Laboratory Group (Thailand) Co.,Ltd. (Rayong Branch)**
		616/10 Moo 5 T.Maenamkoo,
		A.Pluakdaeng, Rayong 21140
Customer Location	:	**ENVIRONMENT LABORATORY**
Date of Receipt	:	**3 September 2025**
Calibrated By	:	**Sujjar Naknakred (Site Calibration Manager)**
Approved By	:	**Boonchai Suriyawong (Site Calibration Manager)**
Date of Issue	:	17 SEP 2025

REVIEW BY Thanitoll.
APPROVED BY
NEXT CAL. DATE 10/03/27

The uncertainties are for a confidence probability of approximately 95%.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standard laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Metrological Center.

Certificate No. T251530

Calibration Report

Equipment : **Chamber (Oven)**
Date of Calibration : **10 September 2025**
Environment : **Temperature : 35.7-36.6 °C**
Line Voltage : 226.8-233.7 V
Relative Humidity : 55 - 65 %RH

Condition of this results of calibration :

1. This equipment was calibrated by insert nine resistance thermometer detectors into its chamber , the other one resistance thermometer detector use for ambient temperature measurement . The calibration was done in according to WI-T20 (based on ASTM E145-94 (Reapproved 2019) and AS2853-1986).
   All data show below were final values and the initial data from customer request . The temperature scale used was based on ITS - 90 .
2. Reference Standard Instrument :

Instrument	Model	Instrument No.	Certificate No.	Due Date
RTD	100 ohm	30-(CH1-10)	T242203	9 November 2025
DATA LOGGER	34970A	T47	T242203	9 November 2025

3. This certificate is traceable to :
   National Institute of Metrology (Thailand) through Metrological Center (NSC-TISI-TIS 17025 CALIBRATION 0244.
4. Condition of calibrated item : good
   Equipment Description :
   Time Constant 3 Hour 29 Minute At 104 °C
   Fresh Air Damper [X] Open [X] Min [ ] Medium [ ] Max
   [ ] Close
   [ ] Not Available
5. Adjustment :
   ( ) without adjustment (X) after adjustment

Approved By

Metrology Center
SCI ECO Services Company Limited
51 Moo 8, Tubkwang, Kaeng Khoi, Saraburi, Thailand 18260

NSC-TISI-TIS 17025
CALIBRATION 0244

Calibration Report

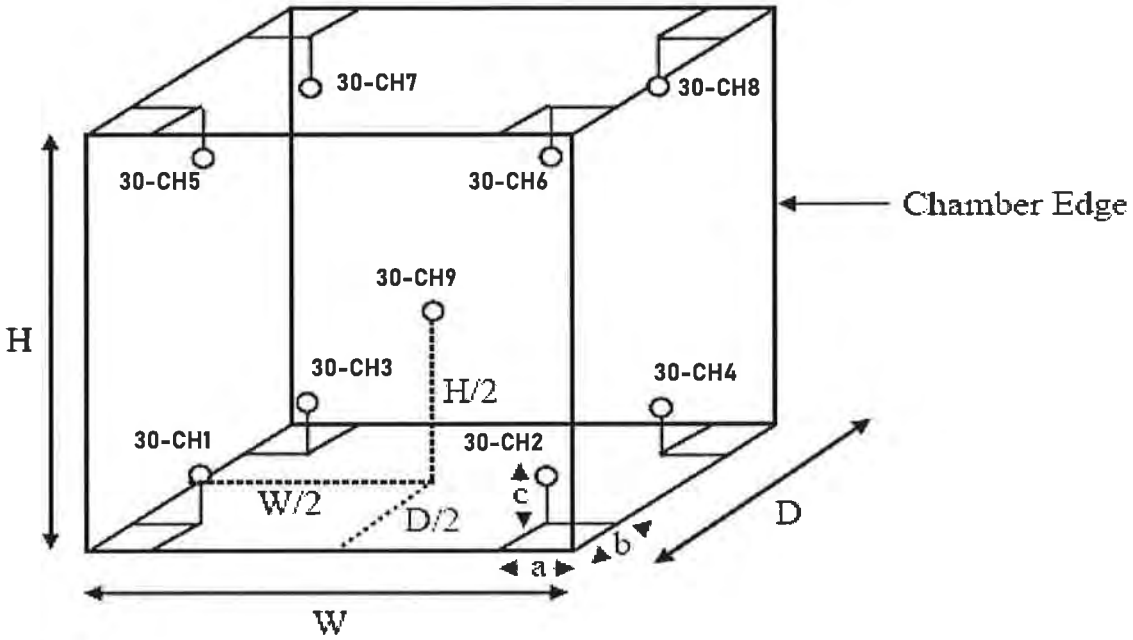

Remark : Internal Dimensions of Chamber : W (Width) = 56 cm. , H (Height) = 48 cm. and D (Depth) = 40 cm.
Size of Installed Standard sensor number 30-CH1 to number 30-CH8 : a = 5 cm. ,b = 5 cm. and c = 5 cm.
Size of Installed Standard sensor number 30-CH9 : W/2 = 56 cm./2 , H/2 = 48 cm./2 and D/2 = 40cm./2

Measurement Results

	Average Standard Reading at each position (°C)								
Calibration Point	30-CH1	30-CH2	30-CH3	30-CH4	30-CH5	30-CH6	30-CH7	30-CH8	30-CH9
104	104.02	103.70	104.01	104.16	104.11	104.08	104.01	104.33	103.61
180	180.67	178.78	180.38	179.85	179.16	180.27	180.98	181.04	179.49

Chamber (Oven)			Temperature Distribution				
Setting °C	Reading (°C)		Average (°C)	Stability (± °C)	Uniformity (°C)	Uncertainty (± °C)	Coverage Factor *k*
	Min , Max	Average					
104.0	103.9 , 104.1	104.0	104.00	0.08	0.61	0.42	2.00
180.0	179.9 , 180.1	180.0	180.07	0.21	1.51	0.52	2.00

* The quoted uncertainty exclude "uniformity"

The calibration result apply only the above calibrated item.

The result of test was found accurate as shown on date and place of test only.

The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor k which for a t-distribution, providing a level of confidence of approximately 95 % .

End of Certificate.

Approved By.

Certificate of Calibration

Represent to Certificate of Calibration No. C29240007

Equipment:	Block Digestion Unit	Certificate No.:	C29240011
Model:	KT-20s	Issued Date:	22 March 2024
Serial No. (or ID.):	5720210009/5770200073	Job No.:	WO-00020429
Manufacturer:	Gerhardt	Page:	1 of 4
Condition:	In Condition	Digestion Block:	20 holes.

Customer: ALS Laboratory Group (Thailand) Co.,Ltd. (Rayong Branch)
616/10 Moo 5 T.Maenam Khu, A.Pluakdaeng, Rayong 21140, Thailand.

Environment Condition:

Temperature:	25 °C	±	0.7 °C
Humidity:	54 %RH	±	4.1 %RH
Voltage:	225 VAC	±	1.7 VAC

REVIEW BY N.Bamrit
APPROVED BY
NEXT CAL. DATE 11/09/25
TKU
16/6/24 ปรับตามวันที่ Cal

Calibration Place: ALS Laboratory Group (Thailand) Co.,Ltd. (Rayong Branch)
(Wet Chemistry Lab)
616/10 Moo 5 T.Maenam Khu, A.Pluakdaeng, Rayong 21140, Thailand.

Calibration By: Mr. Thanathorn Phunook

Calibration Date: *11 March 2024*

The Method used: In house method, base on by comparison with standard

Traceability: This certificate is traceable to the SI Units maintained by National Institute of Metrology (NIMT), Thailand through N.M. Technical Center Laboratory (NTL) Certificate No.: TC22/0080

(Mr. Thanathorn Phunook)
Person in charge

(Mr. Udon Srichana)
Authorized signatory

This certificate is issued the units of measurement according to the International System of Units (SI). It provides traceability of measurement to international or national standard or other recognized national standard laboratories.

The measurement uncertainty stated is the expanded uncertainty which is obtained from the standard uncertainty multiplied by the coverage factor (k=2) to provide a level of confidence of approximately 95%. It is determined in accordance with the Guide to Expression of Uncertainty in Measurement (GUM).

These results may be affected by deviations from specified conditions. The results relate only to the items tested, calibrated or sampled. The report shall not be reproduced except in full without approval of DKSH Technology Limited.

บริษัท ดีเคเอสเอช เทคโนโลยี จำกัด
DKSH Technology Limited
2533 ถนนสุขุมวิท แขวงบางจาก เขตพระโขนง กรุงเทพมหานคร 10260
2533 Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Phone: +66 2639 7000 Email: info.calibration@dksh.com Website: www.dksh.com/scientific-thailand

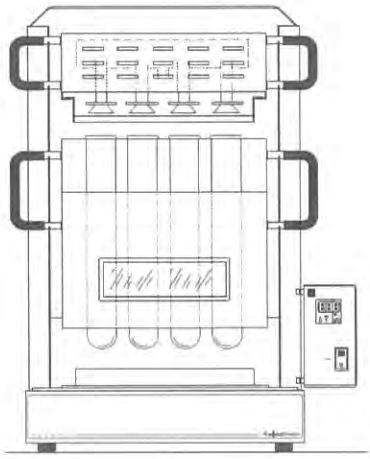

Fig. 1.: Front view

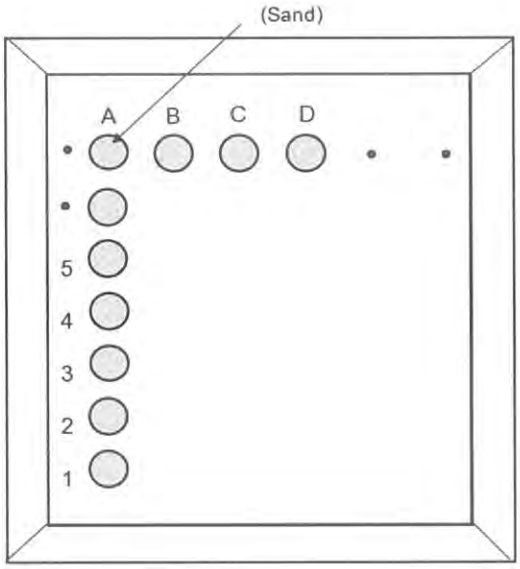

Location of standard

Fig. 2.: Digestion block

Definitions

Indicating Temperature: The average reading of indicating device which forms the integral part of the Digestion block.

Measured Temperature: The average reading of working standard at any positions or location.

Calibration Results:

Pre Calibrtion

Locations	Desired (°C)	Setting (°C)	Indicating (°C)	Measured Temperature (°C)	Correction of UUC. (°C)	Uncertainty (± °C)
A1	380	380	380	401.5	21.5	1.5
A2				401.2	21.2	1.5
A3				399.1	19.1	1.5
A4				397.8	17.8	1.5
A5				395.1	15.1	1.5
B1				396.6	16.6	1.5
B2				396.1	16.1	1.5
B3				392.9	12.9	1.5
B4				391.6	11.6	1.5
B5				390.7	10.7	1.5
C1				395.3	15.3	1.5
C2				395.6	15.6	1.5
C3				392.8	12.8	1.5
C4				391.7	11.7	1.5
C5				390.3	10.3	1.5
D1				397.6	17.6	1.5
D2				396.6	16.6	1.5
D3				395.0	15.0	1.5
D4				394.2	14.2	1.5
D5				393.6	13.6	1.5

บริษัท ดีเคเอสเอช เทคโนโลยี จำกัด
DKSH Technology Limited
2533 ถนนสุขุมวิท แขวงบางจาก เขตพระโขนง กรุงเทพมหานคร 10260
2533 Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Phone: +66 2639 7000 Email: info.calibration@dksh.com Website: www.dksh.com/scientific-thailand

Calibration Results:

Without adjustment

Locations	Desired (°C)	Setting (°C)	Indicating (°C)	Measured Temperature (°C)	Correction of UUC. (°C)	Uncertainty (± °C)
A1	380	365	365	382.5	17.5	1.5
A2				382.4	17.4	1.5
A3				382.1	17.1	1.5
A4				379.7	14.7	1.5
A5				378.3	13.3	1.5
B1				380.1	15.1	1.5
B2				380.1	15.1	1.5
B3				378.5	13.5	1.5
B4				378.3	13.3	1.5
B5				379.1	14.1	1.5
C1				380.1	15.1	1.5
C2				380.1	15.1	1.5
C3				378.9	13.9	1.5
C4				378.2	13.2	1.5
C5				377.3	12.3	1.5
D1				380.5	15.5	1.5
D2				380.6	15.6	1.5
D3				378.1	13.1	1.5
D4				378.7	13.7	1.5
D5				377.7	12.7	1.5

The End of Certificate

บริษัท ดีเคเอสเอช เทคโนโลยี จำกัด
DKSH Technology Limited
2533 ถนนสุขุมวิท แขวงบางจาก เขตพระโขนง กรุงเทพมหานคร 10260
2533 Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Phone: +66 2639 7000 Email: info.calibration@dksh.com Website: www.dksh.com/scientific-thailand

ใบตรวจสอบสภาพเครื่องควบคุมอุณหภูมิ

เลขที่ใบงาน: WO-00020429

ชนิดเครื่องมือ: Block Digestion Unit รุ่น: KT-20s

หมายเลขเครื่อง: 5720210009/5770200073

ตรวจสอบ (รับ)		รายการตรวจเช็ค	ตรวจสอบ (ส่ง)		หมายเหตุ
11 Mar 2024			11 Mar 2024		
ปกติ	ไม่ปกติ		ปกติ	ไม่ปกติ	
		General			
☑	☐	1. สายไฟ	☑	☐	
☑	☐	2. การทำงาน Main Switch	☑	☐	
☑	☐	3. การทำงาน Selector Key	☑	☐	
☑	☐	4. การแสดงผล Display	☑	☐	
☑	☐	5. สภาพ Hole	☑	☐	
☐	☐	6. สภาพฝาปิด	☐	☐	ไม่มี
☑	☐	7. สภาพตัวเครื่อง	☑	☐	
☑	☐	8. สภาวะแวดล้อม ณ สถานที่ตั้งเครื่อง	☑	☐	

ข้อแนะนำ :

Mr. Thanathorn Phunook

Service Engineer

บริษัท ดีเคเอสเอช เทคโนโลยี จำกัด
DKSH Technology Limited
2533 ถนนสุขุมวิท แขวงบางจาก เขตพระโขนง กรุงเทพมหานคร 10260
2533 Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Phone: +66 2639 7000 Email: info.calibration@dksh.com Website: www.dksh.com/scientific-thailand

Delivering Growth – in Asia and Beyond.

Metrology Center

SCI ECO Services Company Limited

51 Moo 8, Tubkwang, Kaeng Khoi, Saraburi, Thailand 18260

Bangkok Tel : +668 9205 6851 , +669 81924 0059

Saraburi Tel : +669 8247 2360

Website : www.scieco.co.th E-Mail : calibrate@scg.co.th

Certificate No. T251529

Certificate of Calibration

Equipment	:	DIGESTION UNIT
Manufacturer	:	Gerhardt, Germany
Model	:	KT - 20S
Serial No.	:	572021009
Customer Code	:	RYG_EN0188
ID No.	:	T6452A5
Customer	:	ALS Laboratory Group (Thailand) Co.,Ltd. (Rayong Branch)
		616/10 Moo 5 T.Maenamkoo,
		A.Pluakdaeng, Rayong 21140
Customer Location	:	ENVIRONMENT LABORATORY
Date of Receipt	:	3 September 2025
Calibrated By	:	Sujjar Naknakred (Site Calibration Manager)
Approved By	:	_____ / Boonchai Suriyawong (Site Calibration Manager)
Date of Issue	:	17 SEP 2025

REVIEW BY Thanitall.

APPROVED BY D.

NEXT CAL. DATE 10/03/27

The uncertainties are for a confidence probability of approximately 95%.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standard laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Metrological Center.

Metrology Center
SCI ECO Services Company Limited
51 Moo 8, Tubkwang, Kaeng Khoi, Saraburi, Thailand 18260

Calibration Report

Equipment	:	**DIGESTION UNIT**
Date of Calibration	:	**10 September 2025**
Environment	:	**Temperature : 21.7 - 24.3 °C**
		Line Voltage : 226.9 - 232.1 V
		Relative Humidity : 55 - 65 %RH

Condition of this results of calibration :

1. This equipment was calibrated by insert four standard thermocouples type S into its chamber , the other one thermocouple type T use for ambient temperature measurement . The calibration was done in according to WI-T10.
2. Reference Standard Instrument :

Instrument	Model	Instrument No.	Certificate No.	Due Date
TC	Type S	M20A1-(CH1-CH4)	T250750	14 May 2026
DATA LOGGER	34970A	T261	T250750	14 May 2026

3. This certificate is traceable to :
   National Institute of Metrology (Thailand) through Metrological Center (NSC-TISI-TIS 17025 CALIBRATION 0244.)
4. Condition of calibrated item : good
   Equipment Description :
   Time Constant 1 Hour 46 Minute At 380 °C
   Fresh Air Damper ☐ Open ☐ Min ☐ Medium ☐ Max
   ☐ Close
   ☒ Not Available
5. Adjustment :
   (X) without adjustment ( ) after adjustment

Approved By. _____

Metrology Center

SCI ECO Services Company Limited

51 Moo 8, Tubkwang, Kaeng Khoi, Saraburi, Thailand 18260

Calibration Report

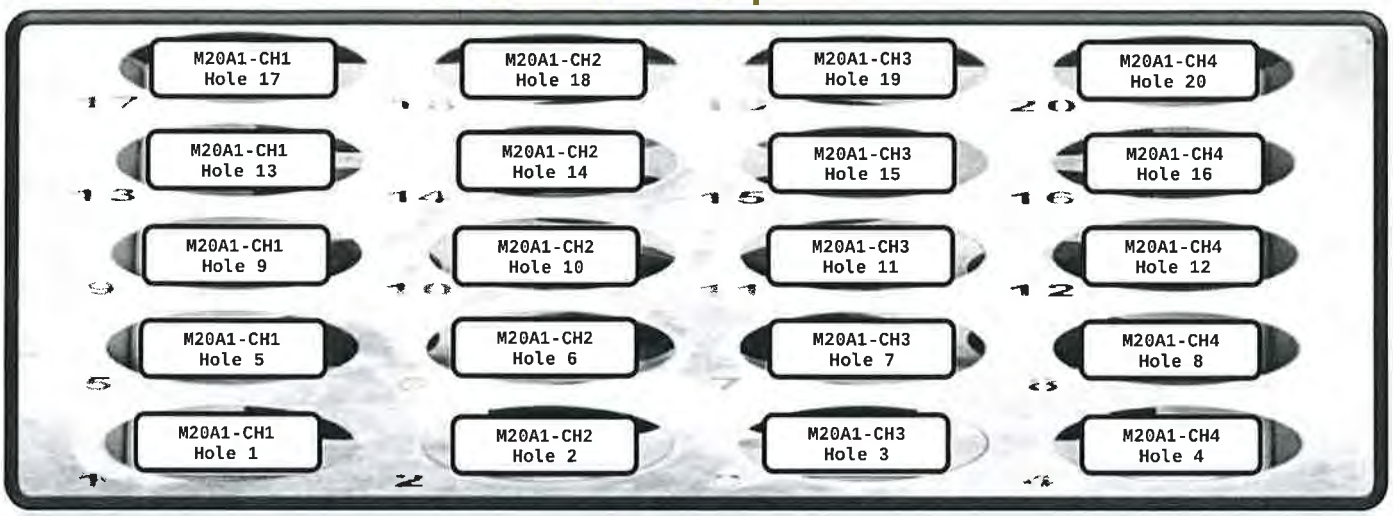

DISPLAY CONTROL (FRONT)

Measurement Results

Cal.Point	Setting	Reading	STD.	Position of Stardards at Block									
(°C)	(°C)	(°C)	Reading	M20A1-CH1 Hole 1	M20A1-CH2 Hole 2	M20A1-CH3 Hole 3	M20A1-CH4 Hole 4	M20A1-CH1 Hole 5	M20A1-CH2 Hole 6	M20A1-CH3 Hole 7	M20A1-CH4 Hole 8	M20A1-CH1 Hole 9	M20A1-CH2 Hole 10
380	360	360	Max °C	381.2	380.5	381.0	381.0	379.2	380.8	381.3	377.7	382.8	381.5
			Mln °C	380.7	380.0	380.4	380.5	378.6	380.1	380.9	377.2	381.9	380.9
			Average °C	381.0	380.3	380.7	380.8	378.9	380.4	381.1	377.5	382.4	381.2
			Stability ±°C	0.3	0.3	0.3	0.2	0.3	0.3	0.2	0.2	0.5	0.3

Cal.Point	Setting	Reading	STD.	Position of Stardards at Block									
(°C)	(°C)	(°C)	Reading	M20A1-CH3 Hole 11	M20A1-CH4 Hole 12	M20A1-CH1 Hole 13	M20A1-CH2 Hole 14	M20A1-CH3 Hole 15	M20A1-CH4 Hole 16	M20A1-CH1 Hole 17	M20A1-CH2 Hole 18	M20A1-CH3 Hole 19	M20A1-CH4 Hole 20
380	360	360	Max °C	382.5	377.2	378.7	378.8	378.5	379.9	383.3	381.0	382.4	381.1
			Min °C	381.7	376.5	378.5	378.5	378.1	379.5	382.7	380.6	381.6	380.4
			Average °C	382.1	376.8	378.6	378.7	378.3	379.7	383.0	380.8	382.0	380.8
			Stability ±°C	0.4	0.4	0.1	0.2	0.2	0.2	0.3	0.2	0.4	0.4

The expanded uncertainty of temperature measurement was ± 1.8 °C

The calibration result apply only the above calibrated item.

The result of test was found accurate as shown on date and place of test only.

The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor k=2 , providing a level of confidence of approximately 95 % .

End of Certificate.

Approved By. _____

Metrology

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110, Thailand.

Saraburi Tel : +66 3627 3096 Fax : +66 3627 3100

Bangkok Tel : +668 9205 6851 , +669 8247 2360

Website : www.scieco.co.th E-Mail : calibrate@scg.com

NSC-TISI-TIS 17025
CALIBRATION 0244

Certificate of Calibration

Equipment	:	Liquid Bath (Water)
Manufacturer	:	Memmert
Model	:	WNE29
Serial No.	:	L623.0105
Customer Code	:	RYG_EN0220
ID No.	:	T5650A5
Customer	:	ALS Laboratory Group (Thailand) Co.,Ltd. (Rayong Branch) 616/10 Moo 5 T.Maenam Khu, A.Pluakdaeng, Rayong 21140
Customer Location	:	Wet Chemistry Lab
Date of Receipt	:	11 December 2024
Calibrated By	:	Atiphong Rongrat (Technician)
Approved By	:	/ Boonchai Suriyawong (Site Calibration Manager)
Date of Issue	:	20 DEC 2024

REVIEW BY ..... ThanitaK.

APPROVED BY.....

NEXT CAL DATE..... 19/12/25

The uncertainties are for a confidence probability of approximately 95%.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standard laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Metrology.

Certificate No. T242075

Calibration Report

Equipment : **Liquid Bath (Water)**

Date of Calibration : **19 December 2024**

Environment : **Temperature : 25.3-25.9 °C**

: **Line Voltage : 221.4-225.4 V**

: **Relative Humidity : 55 - 65 %RH**

Condition of this results of calibration :

1. This equipment was calibrated by insert five resistance thermometer detectors into its water bath , the other one thermocouple type T use for ambient temperature measurement . The calibration was done in according to WI-T36 (based on ASTM E715-80 (Reapproved 2001)).
   All data show below were final values and the initial data from customer request . The temperature scale used, was based on ITS - 90.

2. Reference Standard Instrument :

Instrument	Model	Instrument No.	Certificate No.	Due Date
RTD	100 OHM	M34 (CH1-CH5)	T240400	16 March 2025
DATA LOGGER	34970A	T193	T240400	16 March 2025

3. This certificate is traceable to :
   National Institute of Metrology (Thailand) through Metrological Center (NSC-TISI-TIS 17025 CALIBRATION 0244.)

4. Condition of calibrated item : good
   Equipment Description :
   Time Constar **1** Hour **30** Minute At **63** °C

5. Adjustment :
   (X) without adjustment ( ) after adjustment

Approved By. _____

Certificate No. T242075

Calibration Report

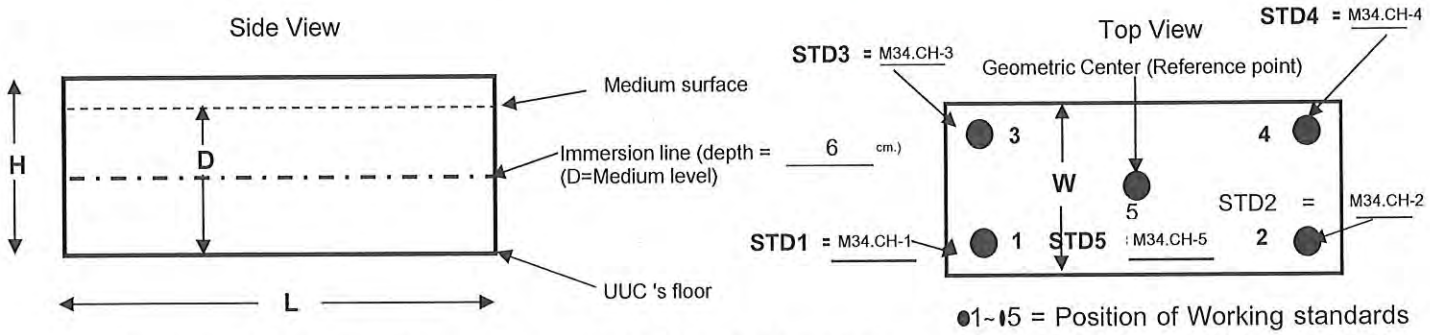

- D = Medium leve 12 cm. Working space dimension : 62 × 42 × 15 (W x L x H)
- UUC 's medium : Water
- Working standards are located : 2.5 cm. away from each coner and walls.

Measurement Results:

	Average Standard Reading at each position (°C)				
Calibration Point	**M34.CH-1**	**M34.CH-2**	**M34.CH-3**	**M34.CH-4**	**M34.CH-5**
63	62.87	63.00	62.88	62.98	63.22
85	84.76	85.14	84.89	85.07	85.24

Liquid Bath (Water)			Temperature Distribution				
Setting (°C)	Reading (°C)		Average (°C)	Stability (±°C)	Uniformity (±°C)	Uncertainty (±°C)	Coverage Factor *k*
	Min , Max	Average					
63.0	-	63.0	62.99	0.07	0.25	0.23	2.00
85.0	-	85.0	85.02	0.13	0.35	0.26	2.00

The calibration result apply only the above calibrated item.

The result of test was found accurate as shown on date and place of test only.

The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor k which for a t-distribution, providing a level of confidence of approximately 95 % .

Approved By. _____

SCG

Metrology Center

SCI ECO Services Company Limited

51 Moo 8, Tubkwang, Kaeng Khoi, Saraburi, Thailand 18260

Bangkok Tel : +668 9205 6851 , +669 81924 0059

Saraburi Tel : +669 8247 2360

Website : www.scieco.co.th E-Mail : calibrate@scg.co.th

NSC-TISI-TIS 17025
CALIBRATION 0244

Certificate No. T252169

Certificate of Calibration

Equipment	:	**Liquid Bath (Water)**
Manufacturer	:	**Memmert**
Model	:	**WNE29**
Serial No.	:	**L623.0105**
Customer Code	:	**RYG_EN0220**
ID No.	:	**T5650A5**
Customer	:	**ALS Laboratory Group (Thailand) Co.,Ltd. (Rayong Branch)**
		616/10 Moo 5 T.Maenamkoo,
		A.Pluakdaeng, Rayong 21140
Customer Location	:	**Wet Chemistry Lab**
Date of Receipt	:	**19 November 2025**
Calibrated By	:	**Sujjar Naknakred (Site Calibration Manager)**
Approved By	:	**/ Boonchai Suriyawong (Site Calibration Manager)**
Date of Issue	:	01 DEC 2025

REVIEW BY Thanitall.
APPROVED BY
NEXT CAL. DATE 27/11/26

The uncertainties are for a confidence probability of approximately 95%.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standard laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Metrological Center.

Certificate No. T252169

Calibration Report

Equipment : **Liquid Bath (Water)**
Date of Calibration : **27 November 2025**
Environment : **Temperature : 25.5-25.7 °C**
Line Voltage : 221.8-225.5 V
Relative Humidity : 55 - 65 %RH

Condition of this results of calibration :

1. This equipment was calibrated by insert five resistance thermometer detectors into its water bath , the other one thermocouple type T use for ambient temperature measurement . The calibration was done in according to WI-T36 (based on ASTM E715-80 (Reapproved 2022)).
   All data show below were final values and the initial data from customer request . The temperature scale used was based on ITS - 90 .
2. Reference Standard Instrument :

Instrument	Model	Instrument No.	Certificate No.	Due Date
RTD	100 OHM	M18 (CH1-CH5)	T251758	17 October 2026
DATA LOGGER	34970A	T261	T251758	17 October 2026

3. This certificate is traceable to :
   National Institute of Metrology (Thailand) through Metrological Center (NSC-TISI-TIS 17025 CALIBRATION 0244.)
4. Condition of calibrated item : good
   Equipment Description :
   Time Constant 1 Hour 3 Minute At 63 °C
5. Adjustment :
   (X) without adjustment ( ) after adjustment

Approved By.

SCG

Metrology Center

SCI ECO Services Company Limited

51 Moo 8, Tubkwang, Kaeng Khoi, Saraburi, Thailand 18260

NSC-TISI-TIS 17025
CALIBRATION 0244

Certificate No. T252169

Calibration Report

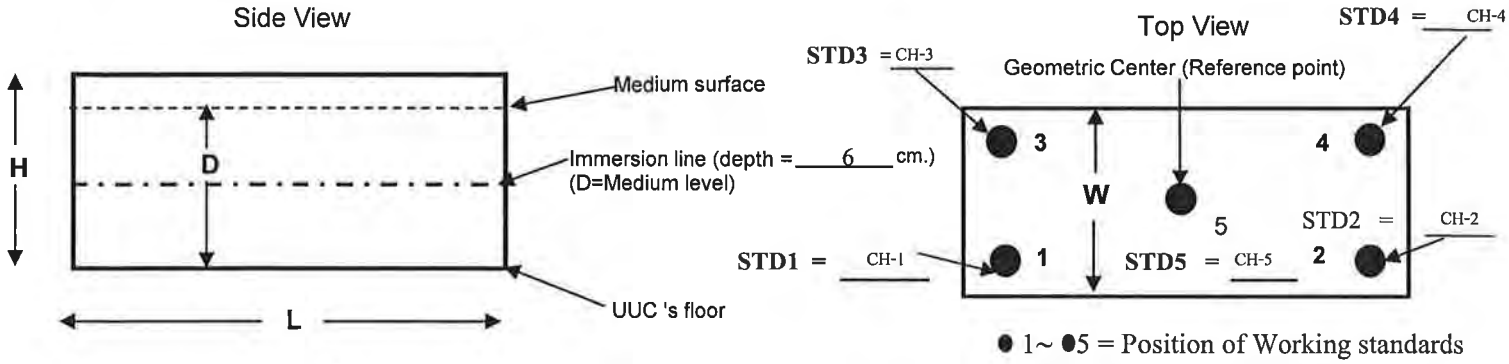

- D = Medium level : 12 cm. Working space dimension : 59 × 35 × 14 (WxLxH)
- UUC 's medium : Water
- Working standards are located at 2.5 cm. away from each coner and walls.

Measurement Results:

	Average Standard Reading at each position (°C)				
Calibration Point	**CH-1**	**CH-2**	**CH-3**	**CH-4**	**CH-5**
63	62.93	63.13	62.94	63.10	63.09
85	85.15	85.33	85.21	85.43	85.20

Liquid Bath (Water)			Temperature Distribution				
Setting (°C)	Reading (°C)		Average	Stability	Uniformity	Uncertainty	Coverage
	Min , Max	Average	(°C)	(±°C)	(±°C)	(±°C)	Factor *k*
63.0	62.9 , 63.1	63.0	63.04	0.08	0.17	0.27	2.06
85.0	84.8 , 85.2	85.0	85.26	0.13	0.24	0.43	2.23

*** The quoted uncertainty exclude "uniformity"**

The calibration result apply only the above calibrated item.

The result of test was found accurate as shown on date and place of test only.

The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor *k* which for a t-distribution, providing a level of confidence of approximately 95 % .

End of Certificate.

Approved By

TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL.0-2717-3000-29 FAX.0-2719-9484

NSC-TISI-TIS17025
CALIBRATION 0008

Certificate of Calibration

Cert.No.: 25CH458
Page.: 1 of 3

Equipment :	pH Meter
Manufacturer :	Mettler Toledo
Model :	Seven2Go S2
Serial No. :	C221115514
ID No. :	RYG_FS0596
Condition As-Received:	Used Item
Received Date :	24 June 2025
Calibration Date :	25 June 2025
Reference :	2506-0782DSC-4
Submitted by :	ALS Laboratory Group (Thailand) Co.,Ltd. Rayong Branch 616/10 Moo 5, T.Maenam Khu, A.Pluakdaeng, Rayong 21140, Thailand
Ambient Temperature :	(25 ± 2.5) °C
Relative Humidity :	(50 ± 15) %
Calibration Procedure :	In - house method : - CP-CH5 by direct measurement with DC voltage standard and direct measurement with certified reference material (CRM) - CP-CH8 by comparison with temperature standard

REVIEW BY Pitthaya T.

APPROVED BY Supt S

NEXT CAL DATE 25/06/26

Calibrated by : Walalak Sirithean

Approved by : Saithip

Approved Signatory

( ) Chakrit Waewwanjua
( ) Ponpan Paipim
(✓) Saithip Meangmai

Issue Date : 26 June 2025

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

Condition of this calibration result

1. Reference Standard Instrument

Instrument	Serial No.	ID No.	Cert. No.	Due Date
1) Document Process Calibrator	54030049	130RC116	24E2759	25 Aug 2025
2) Ref. Standard Thermometer	4982054	110RC044	24I757	14 July 2025

- This measurement result is traceable to SI throught Technology Promotion Association (Thailand - Japan)

2. Certified Reference Materials : The measurement results are traceable to SI through CPA chem Ltd., ANSI-ASQ National Accreditation Board, Accredited No. AR-1835

Buffer Solution	Manufacturer	Lot No.	Exp. date
pH 4.007	CPA chem	1066665	18 Jan 2027
pH 6.965	CPA chem	1066667	18 Jan 2026
pH 10.010	CPA chem	1114385	08 June 2026

3. This certificate is valid only to the item calibrated on date and place of calibration.

Calibration Results

Function : mV Measurement

Performing standard curve by Document Process Calibrator at pH (4,7,10)

Unit Under Calibration	Nominal Value	Standard Voltage Input	Actual Reading		Uncertainty of Measurement (±mV)	Coverage factor *k*
	pH	mV	mV	pH		
pH Meter	4.00	177.48	178	4.00	0.58	2.00
S/N.: C221115514	7.00	0.00	0	7.00	0.58	2.00
	10.00	-177.48	-178	10.00	0.58	2.00

Calibration Results

Function : pH Measurement

Performing three buffers standard curve by using buffer nominal pH (4,7,10)

Unit Under Calibration	Standard pH Buffer Solution	Actual pH Reading	Actual mV Reading (mV)	Uncertainty of pH Measurement (±)	Coverage factor *k*
pH Electrode	4.007	4.01	163	0.0079	2.00
S/N.: 3293232	6.965	6.99	-10	0.011	2.00
	10.010	10.00	-185	0.0092	2.00

Function : Temperature Measurement

(*) Without adjustment

This equipment was connected with Temperature Probe;

- Model : InLabExpert Go-ISM
- Serial No. : 3293232

Dimension of probe

- Length : 120 mm.
- Diameter : 12 mm.
- Immersion Depth : 100 mm.

Calibration Point (°C)	Standard Temperature (°C)	UUC* Reading (°C)	Error (°C)	Uncertainty of measurement (± °C)	Coverage factor *k*
25.0	25.002	25.1	0.098	0.13	2.00
45.0	45.001	45.2	0.199	0.13	2.00

Remark - UUC* = Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

SCG

Metrology

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110, Thailand.

Saraburi Tel : +66 3627 3096 Fax : +66 3627 3100

Bangkok Tel : +668 9205 6851 , +669 8247 2360

Website : www.scieco.co.th E-Mail : calibrate@scg.com

NSC-TISI-TIS 17025
CALIBRATION 0244

Certificate No. T241120

Certificate of Calibration

Equipment	:	**Chamber (Cold Room)**
Manufacturer	:	**MODULAR**
Model	:	**IREVCOHCOO**
Serial No.	:	**C00351459**
Customer Code	:	**RYG_EN0184**
ID No.	:	**T1939A5**
Customer	:	**ALS Laboratory Group (Thailand) Co.,Ltd. (Rayong Branch)**
		616/10 Moo 5 T.Maenam Khu,
		A.Pluakdaeng, Rayong 21140
Customer Location	:	**Laboratory**
Date of Receipt	:	**5 June 2024**
Calibrated By	:	**Sujjar Naknakred (Site Calibration Manager)**
Approved By	:	**Preecha Phisassutthikul (Temperature Calibration Manager)**
Date of Issue	:	12 JUN 2024

REVIEW BY Thanitall.
APPROVED BY
NEXT CAL. DATE 11/12/25

The uncertainties are for a confidence probability of approximately 95%.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standard laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Metrology.

Certificate No. T241120

Calibration Report

Equipment : **Chamber (Cold Room)**
Date of Calibration : **11 June 2024**
Environment : **Temperature : 23.1-24.1 °C**
Line Voltage : 222.3-226.3 V
Relative Humidity : 55 - 65 %RH

Condition of this results of calibration :

1. This equipment was calibrated by insert nine standard thermocouples type T into its chamber , the other one standard thermocouples type T use for ambient temperature measurement . The calibration was done in according to WI-T20 (based on ASTM E145-94 (Reapproved 2001) and AS2853-1986).
   All data show below were final values and the initial data from customer request . The temperature scale used was based on ITS - 90 .
2. Reference Standard Instrument :

Instrument	Model	Instrument No.	Certificate No.	Due Date
TC	TYPE T	TN161-TN170	T240713	19 April 2025
TC	TYPE T	TN171-TN180	T240713	19 April 2025
DATA LOGGER	34970A	T149	T240713	19 April 2025

3. This certificate is traceable to :
   National Institute of Metrology (Thailand) through Metrological Center (NSC-TISI-TIS 17025 CALIBRATION 0244.)
4. Condition of calibrated item : good
   Equipment Description :
   Time Constant 3 Hour 30 Minute At 3 °C
   Fresh Air Damper ☐ Open ☐ Min ☐ Medium ☐ Max
   ☐ Close
   ☒ Not Available
5. Adjustment :
   ( ) without adjustment (X) after adjustment

Approved By_____

Certificate No. T241120

Calibration Report

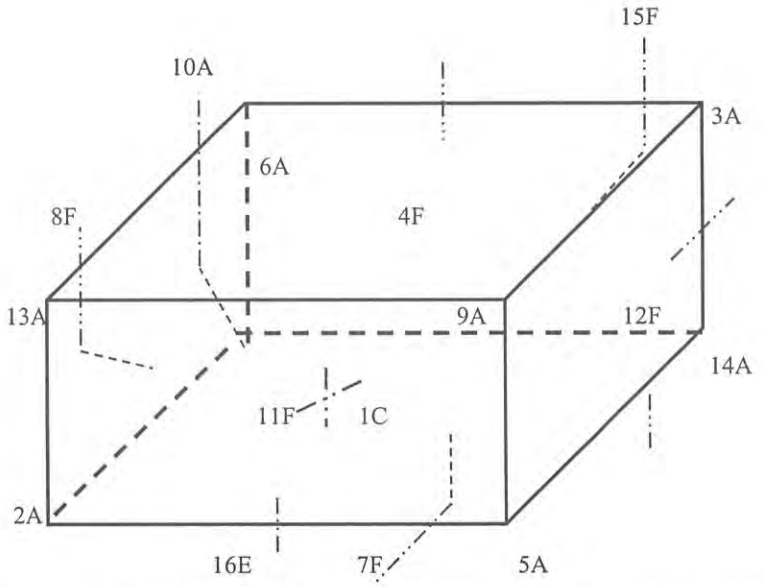

C = Centre , F = Centre of Face , A = Corner , E = Centre of Edge

1C	=	TN161
2A	=	TN162
3A	=	TN163
4F	=	TN164
5A	=	TN165
6A	=	TN166
7F	=	TN167
8F	=	TN168
9A	=	TN169
10A	=	TN170

11F	=	TN171
12F	=	TN172
13A	=	TN173
14A	=	TN174
15F	=	TN175
16E	=	TN176

Approved By.

Certificate No. T241120

Calibration Report

Measurement Results:

	Average Standard Reading at each position (°C)									
Calibration Point	**TN161**	**TN162**	**TN163**	**TN164**	**TN165**	**TN166**	**TN167**	**TN168**	**TN169**	**TN170**
3	2.73	2.70	2.77	2.78	2.99	2.35	3.09	3.21	3.08	2.90
	TN171	**TN172**	**TN173**	**TN174**	**TN175**	**TN176**				
	3.39	3.01	2.92	2.81	3.42	3.42				

Chamber (Cold Room)			Temperature Distribution				
Setting (°C)	Reading (°C)		Average (°C)	Stability (±°C)	Uniformity (°C)	Uncertainty (±°C)	Coverage Factor *k*
	Min , Max	Average					
3.0	2.9 , 4.4	3.7	2.97	1.32	1.13	2.02	2.00

* The quoted uncertainty exclude " uniformity "

The calibration result apply only the above calibrated item.

The result of test was found accurate as shown on date and place of test only.

The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor *k* which for a t-distribution, providing a level of confidence of approximately 95 % .

Approved By. _____

SCG

Metrology Center

SCI ECO Services Company Limited

51 Moo 8, Tubkwang, Kaeng Khoi, Saraburi, Thailand 18260

Bangkok Tel : +668 9205 6851 , +669 81924 0059

Saraburi Tel : +669 8247 2360

Website : www.scieco.co.th E-Mail : calibrate@scg.co.th

NSC-TISI-TIS 17025
CALIBRATION 0244

Certificate No. T252167

Certificate of Calibration

Equipment	:	**Chamber (Cold Room)**
Manufacturer	:	**MODULAR**
Model	:	**IREVCOHCOO**
Serial No.	:	**C00351459**
Customer Code	:	**RYG_EN0184**
ID No.	:	**T1939A5**
Customer	:	**ALS Laboratory Group (Thailand) Co.,Ltd. (Rayong Branch)** **616/10 Moo 5 T.Maenamkoo,** **A.Pluakdaeng, Rayong 21140**
Customer Location	:	**ENVIRONMENT LABORATORY**
Date of Receipt	:	**19 November 2025**
Calibrated By	:	**Sujjar Naknakred (Site Calibration Manager)**
Approved By	:	**/ Boonchai Suriyawong (Site Calibration Manager)**
Date of Issue	:	01 DEC 2025

REVIEW BY Thanitall.
APPROVED BY
NEXT CAL. DATE 27/05/27

The uncertainties are for a confidence probability of approximately 95%.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standard laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Metrological Center.

Certificate No. T252167

Calibration Report

Equipment : **Chamber (Cold Room)**
Date of Calibration : **27 November 2025**
Environment : **Temperature : 24.7-25.6 °C**
Line Voltage : 222.3-226.3 V
Relative Humidity : 55 - 65 %RH

Condition of this results of calibration :

1. This equipment was calibrated by insert nine standard thermocouples type T into its chamber , the other one standard thermocouples type T use for ambient temperature measurement . The calibration was done in according to WI-T20 (based on ASTM E145-94 (Reapproved 2019) and AS2853-1986).
   All data show below were final values and the initial data from customer request . The temperature scale used was based on ITS - 90 .
2. Reference Standard Instrument :

Instrument	Model	Instrument No.	Certificate No.	Due Date
TC	TYPE T	TN161-TN170	T251760	17 October 2026
TC	TYPE T	TN171-TN180	T251760	17 October 2026
DATA LOGGER	34970A	T261	T251760	17 October 2026

3. This certificate is traceable to :
   National Institute of Metrology (Thailand) through Metrological Center (NSC-TISI-TIS 17025 CALIBRATION 0244.)
4. Condition of calibrated item : good
   Equipment Description :
   Time Constant 1 Hour 12 Minute At 3 °C
   Fresh Air Damper ☐ Open ☐ Min ☐ Medium ☐ Max
   ☐ Close
   ☒ Not Available
5. Adjustment :
   ( ) without adjustment (X) after adjustment

Approved By._____

Certificate No. T252167

Calibration Report

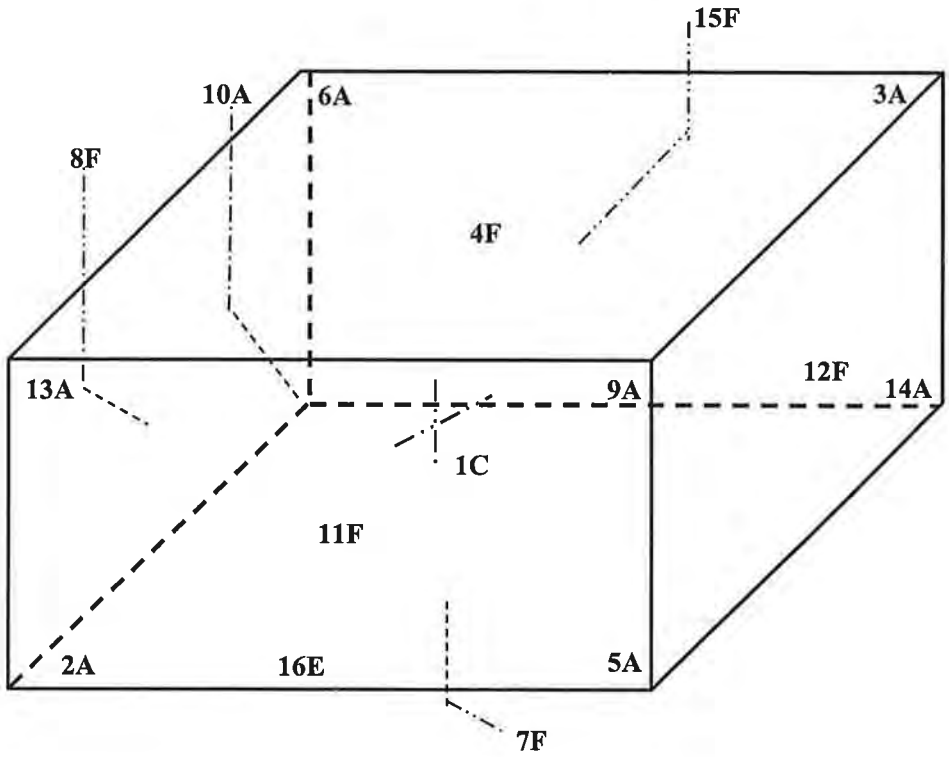

C = Centre , F = Centre of Face , A = Corner , E = Centre of Edge

1C	=	TN161
2A	=	TN162
3A	=	TN163
4F	=	TN164
5A	=	TN165
6A	=	TN166
7F	=	TN167
8F	=	TN168
9A	=	TN169
10A	=	TN170

11F	=	TN171
12F	=	TN172
13A	=	TN173
14A	=	TN174
15F	=	TN175
16E	=	TN176

Approved By._____

SCG

Metrology Center

SCI ECO Services Company Limited

51 Moo 8, Tubkwang, Kaeng Khoi, Saraburi, Thailand 18260

NSC-TISI-TIS 17025
CALIBRATION 0244

Certificate No. T252167

Calibration Report

Measurement Results:

Calibration Point	Average Standard Reading at each position (°C)									
	1C TN161	2A TN162	3A TN163	4F TN164	5A TN165	6A TN166	7F TN167	8F TN168	9A TN169	10A TN170
3	2.59	2.80	2.94	2.86	3.05	3.44	3.11	3.30	3.29	3.66
	11F TN171	12F TN172	13A TN173	14A TN174	15F TN175	16E TN176				
	3.41	3.56	3.38	3.54	3.36	3.16				

Chamber (Cold Room)			Temperature Distribution				
Setting (°C)	Reading (°C)		Average (°C)	Stability(±°C)	Uniformity(°C)	Uncertainty(±°C)	Coverage Factor *k*
	Min , Max	Average					
3.0	2.9 , 4.1	3.7	3.21	1.25	1.92	1.85	2.00

* The quoted uncertainty exclude " uniformity "

The calibration result apply only the above calibrated item.

The result of test was found accurate as shown on date and place of test only.

The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor *k* which for a t-distribution, providing a level of confidence of approximately 95 % .

End of Certificate.

Approved By. _____

DKSH

NSC-TISI-TIS 17025
Calibration 0087

Certificate of Calibration

Equipment:	CONDUCTIVITY METER		Certificate No.:	C24250077	
Model:	Orion STAR A215		Issued Date:	21 March 2025	
Serial No. (or ID.):	X58821 (RYG-EN0200)		Job No.:	WO-00064803	
Manufacturer:	Thermo Scientific		Page:	1 of 2	
Electrode Serial No.	YQ1-11982	Model :	ORION 013005MD	Brand :	Thermo Scientific
Condition:	In Condition				

Customer: ALS Laboratory Group (Thailand) Co.,Ltd. (Rayong Branch)
616/10 Moo 5 T.Maenam Khu,
A.Pluakdaeng, Rayong 21140, Thailand.

REVIEW BY Photchanan S.
APPROVED BY D. Suradech
NEXT CAL. DATE 21/3/26

Environment Condition:	Temperature	23.5	°C	±	0.8	°C
	Humidity	52.4	%RH	±	1.3	%RH

Calibration Place: ALS Laboratory Group (Thailand) Co.,Ltd. (Rayong Branch)
(Wet Chemisty Lab) 616/10 Moo 5 T.Maenam Khu,
A.Pluakdaeng, Rayong 21140, Thailand.

Calibration By: Mr. Pongpisut Suebchantha

Calibration Date: 21 March 2025

The Method used: In house method, CAL-WI-49, base on ASTM D 1125-14 and D 5391-14

Traceability: This certificate is traceable to the SI Units maintained by CRM of NIST(SRM) through CPA chem Co., Ltd. (ISO/IEC 17034) Certificate No. 1066606, 1066607, 1066608, 1066609

(Mr. Pongpisut Suebchantha)
Person in charge

(Miss Kaewkan Suradech)
Authorized signatory

This certificate is issued the units of measurement according to the International System of Units (SI). It provides traceability of measurement to international or national standard or other recognized national standard laboratories.

The measurement uncertainty stated is the expanded uncertainty which is obtained from the standard uncertainty multiplied by the coverage factor (k=2) to provide a level of confidence of approximately 95%. It is determined in accordance with the Guide to Expression of Uncertainty in Measurement (GUM).

These results may be affected by deviations from specified conditions. The results relate only to the items tested, calibrated or sampled. The report shall not be reproduced except in full without approval of DKSH Technology Limited.

บริษัท ดีเคเอสเอช เทคโนโลยี จำกัด
DKSH Technology Limited
2533 ถนนสุขุมวิท แขวงบางจาก เขตพระโขนง กรุงเทพมหานคร 10260
2533 Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Phone: +66 2639 7000 Email: info.calibration@dksh.com Website: www.dksh.com/scientific-thailand

Calibration Results:

Before Adjustment

Standard Conductivity Solution		Unit Under Calibration Reading		Correction		Coverage Factor (k)	Uncertainty (±)	
25.000	µS/cm	27.43	µS/cm	-2.430	µS/cm	2.00	0.28	µS/cm
84.003	µS/cm	90.76	µS/cm	-6.757	µS/cm	2.00	0.68	µS/cm
1413.1	µS/cm	1464	µS/cm	-50.9	µS/cm	2.00	11	µS/cm
12.881	mS/cm	13.41	mS/cm	-0.529	mS/cm	2.00	0.098	mS/cm

After Adjustment ; at 25 µS/cm, 84 µS/cm, 1413 µS/cm, 12.88 mS/cm

Standard Conductivity Solution		Unit Under Calibration Reading		Correction		Coverage Factor (k)	Uncertainty (±)	
25.000	µS/cm	25.63	µS/cm	-0.630	µS/cm	2.00	0.28	µS/cm
84.003	µS/cm	84.53	µS/cm	-0.527	µS/cm	2.00	0.68	µS/cm
1413.1	µS/cm	1415	µS/cm	-1.9	µS/cm	2.00	11	µS/cm
12.881	mS/cm	12.92	mS/cm	-0.039	mS/cm	2.00	0.098	mS/cm

The End of Certificate

บริษัท ดีเคเอสเอช เทคโนโลยี จำกัด
DKSH Technology Limited
2533 ถนนสุขุมวิท แขวงบางจาก เขตพระโขนง กรุงเทพมหานคร 10260
2533 Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Phone: +66 2639 7000 Email: info.calibration@dksh.com Website: www.dksh.com/scientific-thailand

ใบตรวจสอบสภาพเครื่องวัดสิ่งแวดล้อม

เลขที่ใบงาน: WO-00064803

ชนิดเครื่องมือ: CONDUCTIVITY METER รุ่น: Orion STAR A215 หมายเลขเครื่อง: X58821

ตรวจสอบ (รับ) 21 Mar 2025 ปกติ	ตรวจสอบ (รับ) 21 Mar 2025 ไม่ปกติ	รายการตรวจเช็ค	ตรวจสอบ (ส่ง) 21 Mar 2025 ปกติ	ตรวจสอบ (ส่ง) 21 Mar 2025 ไม่ปกติ	หมายเหตุ
		General			
☑	☐	1. ความสมบูรณ์เครื่อง	☑	☐	
☑	☐	2. ความสะอาด (ช่องใส่ตัวอย่าง, ภายใน-นอกเครื่อง)	☑	☐	
☑	☐	3. สวิทช์ ปิด – เปิด เครื่อง (On-Off Swicth)	☑	☐	
☑	☐	4. ปุ่มกด (Keypad)	☑	☐	
☑	☐	5. หน้าจอ (Display, Screen Contrast)	☑	☐	
		Spectrophotometer			
☐	☐	6. แรงดันไฟฟ้า (Battery Backup) >= 2.5 VDC	☐	☐	
☐	☐	7. ตัวหมุนเลือกความยาวคลื่น (Wavelength Control)	☐	☐	
☐	☐	8. ความยาวคลื่น (Wavelength Check)	☐	☐	
☐	☐	9. แหล่งกำเนิดแสง (UV < 3,000 hour)	☐	☐	
☐	☐	10. แหล่งกำเนิดแสง (Visible < 5,000 hour)	☐	☐	
☐	☐	11. ช่องวัดหลายตัวอย่าง (Carousel Module)	☐	☐	
		pH Meter and Conductivity Meter			
☑	☐	12. อิเล็คโทรด (Electrode and Connection Cable)	☑	☐	
☐	☐	13. ระดับสารละลายใน Electrode (Level KCl)	☐	☐	
☐	☐	14. ฝาปิดกันปลาย Electrode (Dust Protection Hood)	☐	☐	
☑	☐	15. ขาจับอิเล็คโทรด (Stand)	☑	☐	
		Turbidimeter			
☐	☐	16. ค่าความขุ่นที่ต่ำสุด (No Sample)	☐	☐	
☐	☐	17. ระดับการส่องสว่างของแสง (>= 2.5 ไม่เกิน 3.0)	☐	☐	
		Automatic titrator			
☐	☐	18. สภาพ Piston Burettes	☐	☐	
☐	☐	19. Function Rinsing and Dosing	☐	☐	
☐	☐	20. ระบบท่อสายยางและอุปกรณ์ประกอบ	☐	☐	

ข้อแนะนำ : _____

Mr. Pongpisut Suebchantha

Service Engineer

บริษัท ดีเคเอสเอช เทคโนโลยี จำกัด
DKSH Technology Limited
2533 ถนนสุขุมวิท แขวงบางจาก เขตพระโขนง กรุงเทพมหานคร 10260
2533 Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Phone: +66 2639 7000 Email: info calibration@dksh.com Website: www.dksh.com/scientific-thailand

Delivering Growth – in Asia and Beyond.

DKSH

NSC-TISI-TIS 17025
Calibration 0087

Certificate of Calibration

Equipment : Digital Thermometer with Probe
Model : Orion STAR A215
Serial No. : X58821
Manufacturer : Thermo Scientific
ID No. : RYG-EN0200

Certificate No. : C15250430
Issued Date : 21 March 2025
Job No. : WO-00064803

Condition : In Condition

Customer : ALS Laboratory Group (Thailand) Co.,Ltd. (Rayong Branch)
616/10 Moo 5 T.Maenam Khu,
A.Pluakdaeng, Rayong 21140, Thailand.

REVIEW BY Photchanan S.
APPROVED BY
NEXT CAL. DATE 21/3/26

Environment Condition :

Temperature:	30 °C	±	10 °C
Humidity:	55 %RH	±	25 %RH
Voltage:	220 VAC	±	10 %

Calibration Place : ALS Laboratory Group (Thailand) Co.,Ltd. (Rayong Branch)
(Wet Chemistry Lab) 616/10 Moo 5 T.Maenam Khu,
A.Pluakdaeng, Rayong 21140, Thailand.

Calibration By : Mr. Piyapat Saidoung
Calibration Date : 21 March 2025
The Method used : In house method, CAL-WI-69, by comparison with standard thermometer
Traceability : This certificate is traceable to the International System of Unit maintained by:
Quality Reborn Co.,Ltd. (QR)

(Mr. Piyapat Saidoung)
Person in charge

(Mr. Tweewong Thaithiang)
Authorized signatory

This certificate is issued the units of measurement according to the International System of Units (SI). It provides traceability of measurement to international or national standard or other recognized national standard laboratories.

The measurement uncertainty stated is the expanded uncertainty which is obtained from the standard uncertainty multiplied by the coverage factor (k=2) to provide a level of confidence of approximately 95%. It is determined in accordance with the Guide to Expression of Uncertainty in Measurement (GUM).

These results may be affected by deviations from specified conditions. The results relate only to the items tested, calibrated or sampled. The report shall not be reproduced except in full without approval of DKSH Technology Limited.

บริษัท ดีเคเอสเอช เทคโนโลยี จำกัด
DKSH Technology Limited
2533 ถนนสุขุมวิท แขวงบางจาก เขตพระโขนง กรุงเทพมหานคร 10260
2533 Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Phone: +66 2639 7000 Email: info.calibration@dksh.com Website: www.dksh.com/scientific-thailand

Reference standard equipment:

Equipment	Certificate no	Cal. date	Next Cal. date
Digital Thermometer with Probe	QR24-2043	21 August 2024	21 August 2025

Calibration Results:

Without Adjustment

Sensor Type: RTD Electrode Serial No. CS1-11923 Channel: -

Diameter (mm): 15 Length (mm): 120 Immersion (mm): 110

Calibrate Point.(°C)	STD. Reading (°C)	UUC. Reading (°C)	Correction of UUC (°C)	Uncertainty (± °C)
25.0	24.954	24.9	0.054	0.20

The End of Certificate

บริษัท ดีเคเอสเอช เทคโนโลยี จำกัด
DKSH Technology Limited
2533 ถนนสุขุมวิท แขวงบางจาก เขตพระโขนง กรุงเทพมหานคร 10260
2533 Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Phone: +66 2639 7000 Email: info.calibration@dksh.com Website: www.dksh.com/scientific-thailand

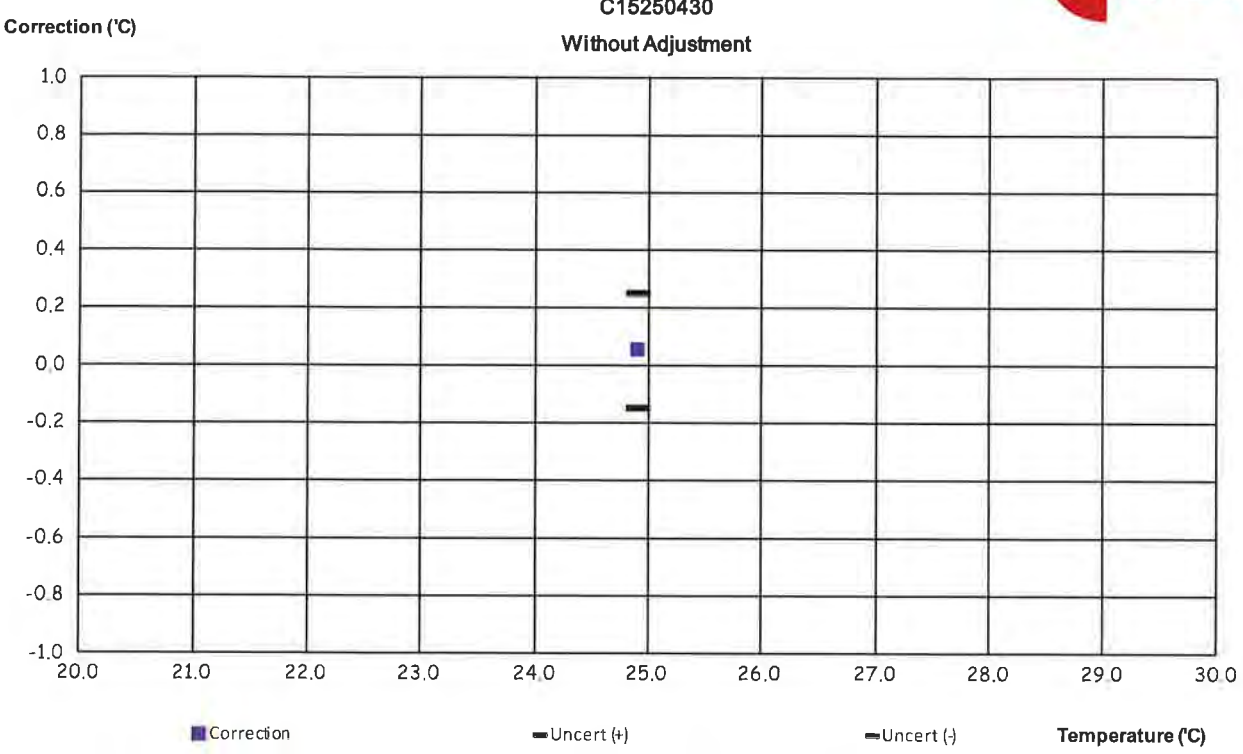
C15250430
Without Adjustment
Correction ('C)
1.0
0.8
0.6
0.4
0.2
0.0
-0.2
-0.4
-0.6
-0.8
-1.0
20.0
21.0
22.0
23.0
24.0
25.0
26.0
27.0
28.0
29.0
30.0
Correction
Uncert (+)
Uncert (-)
Temperature ('C)

ใบตรวจสอบสภาพเครื่องมือวัดอุณหภูมิ

Equipment : Digital Thermometer with Probe

Certificate No. : C15250430

Serial No. : X58821

Model : Orion STAR A215

ตรวจสอบ (รับ)		รายการตรวจเช็ค	ตรวจสอบ (ส่ง)		หมายเหตุ
21-Mar-2025			21-Mar-2025		
ปกติ	ไม่ปกติ		ปกติ	ไม่ปกติ	
		General			
☑	☐	1. สายไฟ	☑	☐	
☑	☐	2. Adapter / Power supply 220 / 110 VAC	☑	☐	
☑	☐	3. การทำงาน Main Switch	☑	☐	
☑	☐	4. การทำงาน Selector Key	☑	☐	
☑	☐	5. การแสดงผล Display	☑	☐	
☐	☐	6. Battery	☐	☐	ไม่มี
☑	☐	7. สภาพตัวเครื่อง	☑	☐	
☑	☐	8. สภาพ Sensor (In / Ex)	☑	☐	

ข้อแนะนำ : _____

_____

_____

Mr. Piyapat Saidoung

Service Engineer

บริษัท ดีเคเอสเอช เทคโนโลยี จำกัด
DKSH Technology Limited
2533 ถนนสุขุมวิท แขวงบางจาก เขตพระโขนง กรุงเทพมหานคร 10260
2533 Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Phone: +66 2639 7000 Email: info.calibration@dksh com Website: www.dksh.com/scientific-thailand

Delivering Growth – in Asia and Beyond.

TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL.0-2717-3000-29 FAX.0-2719-9484

NSC-TISI-TIS17025
CALIBRATION 0008

Certificate of Calibration

Cert.No.: 24CHO568
Page.: 1 of 3

Equipment :	Spectrophotometer
Manufacturer :	HACH
Model :	DR3900
Serial No. :	2021559
ID No. :	BKK_EN0356
Condition As-Received:	Used Item
Received Date :	29 October 2024
Calibration Date :	29 October 2024
Reference :	2410-0782OC-1
Submitted by :	ALS Laboratory Group (Thailand) Co.,Ltd. 104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan, Khet Suan Luang, Bangkok 10250 Thailand
Calibration Place :	Wet Chemistry Lab 2
Ambient Temperature :	(21.8 to 21.5) °C (On-Site)
Relative Humidity :	(58.2 to 59.3) % (On-Site)
Calibration Procedure :	In - house method : CP-OCH4 based on ASTM E 275-08
Calibrated by :	Warakorn Lerngagtrakul
Approved by :	Saithip Approved Signatory

REVIEW BY ..... Sinda K .....
APPROVED BY ..... Siriluk P. .....
NEXT CAL DATE..... 29/10/25 .....

( ) Unnopphol Harachai
( ) Ponpan Paipim
(✓) Saithip Meangmai

Issue Date : 30 October 2024

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

Condition of calibration result

1. Reference Standard Material :

Material	Serial No.	Certificate No.	Due date
1. Absorbance Standard set	44487	122584	31 May 2026
2. Wavelength Standard set	36730	118120	15 Jan 2026
3. Wavelength Standard set	36730	118121	15 Jan 2026

2. This certificate is valid only to the item calibrated on date and place of calibration.
3. This certificate is traceable to the International System of Unit maintained through :
   - Starna Scientific Ltd.
4. Spectral BandWidth : 5 nm
   Scan Speed : - nm/min

Calibration Results : without adjustment

Wavelength Accuracy

Certified Values of Reference Material (nm)	UUC Reading (nm)	Uncertainty of Measurement (± nm)	Coverage Factor *k*
418.40	418	0.59	2.00
479.88	480	0.59	2.00
513.75	514	0.59	2.00
537.00	536	0.59	2.00
638.00	638	0.59	2.00
747.61	748	0.59	2.00
807.04	808	0.72	2.05

Calibration Results : without adjustment

Photometric Accuracy

Wavelength (nm)	Certified Values of Reference Material (Abs)	UUC Reading (Abs)	Uncertainty of Measurement (±Abs)	Coverage Factor *k*
420.0	Zero	0.000	0.0028	2.00
	0.5750	0.575	0.0028	2.00
	0.7156	0.713	0.0028	2.00
	1.0176	1.015	0.0028	2.00
440.0	Zero	0.000	0.0028	2.00
	0.5598	0.560	0.0028	2.00
	0.7037	0.701	0.0028	2.00
	1.0013	0.998	0.0028	2.00
465.0	Zero	0.000	0.0028	2.00
	0.5222	0.524	0.0028	2.00
	0.6646	0.665	0.0028	2.00
	0.9444	0.945	0.0028	2.00
546.1	Zero	0.000	0.0028	2.00
	0.5234	0.525	0.0029	2.00
	0.7007	0.701	0.0028	2.00
	0.9992	1.000	0.0028	2.00
590.0	Zero	0.000	0.0028	2.00
	0.5573	0.558	0.0029	2.00
	0.7760	0.774	0.0028	2.00
	1.1104	1.108	0.0028	2.00
635.0	Zero	0.000	0.0028	2.00
	0.5648	0.566	0.0029	2.00
	0.7654	0.765	0.0028	2.00
	1.0961	1.096	0.0028	2.00

Remark

- Each individual filter is measured against the empty filter holder (blank) used to zero the spectrophotometer
- * : Not NSC-ONSC Accredited
- UUC = Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k* , providing a level of confidence of approximately 95 %.

-o0o-

TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL.0-2717-3000-29 FAX.0-2719-9484

NSC-TISI-TIS17025
CALIBRATION 0008

Certificate of Calibration

Cert.No.: 25CHO537
Page.: 1 of 3

Equipment :	Spectrophotometer
Manufacturer :	HACH
Model :	DR3900
Serial No. :	2021559
ID No. :	BKK_EN0356
Condition As-Received:	Used Item
Received Date :	08 October 2025
Calibration Date :	08 October 2025
Reference :	2510-0042OC-11
Submitted by :	ALS Laboratory Group (Thailand) Co.,Ltd. 104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan, Khet Suan Luang, Bangkok 10250 Thailand
Calibration Place :	Wet Chemistry Lab 2
Ambient Temperature :	(21.9 to 21.9) °C (On-Site)
Relative Humidity :	(62 to 65) % (On-Site)
Calibration Procedure :	In - house method : CP-OCH4 based on ASTM E 275-08

REVIEW BY ..... Sirida K.

APPROVED BY ..... Siriluk P.

NEXT CAL DATE 08/10/26

Calibrated by : Uthen Kankawi

Approved by : Saithip

Approved Signatory

( ) Chakrit Waewwanjua
( ) Ponpan Paipim
(✓) Saithip Meangmai

Issue Date : 9 October 2025

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

Condition of calibration result

1. Reference Standard Material :

Material	Serial No.	Certificate No.	Due date
1. Absorbance Standard set	44487	122584	31 May 2026
2. Wavelength Standard set	36730	118120	15 Jan 2026
3. Wavelength Standard set	36730	118121	15 Jan 2026

2. This certificate is valid only to the item calibrated on date and place of calibration.
3. This certificate is traceable to the International System of Unit maintained through :
   - Starna Scientific Ltd.
4. Spectral BandWidth : 5 nm
   Scan Speed : - nm/min

Calibration Results : without adjustment

Wavelength Accuracy

Certified Values of Reference Material (nm)	UUC Reading (nm)	Uncertainty of Measurement (± nm)	Coverage Factor *k*
418.40	418	0.59	2.00
479.88	480	0.59	2.00
513.75	513	0.59	2.00
537.00	536	0.59	2.00
638.00	638	0.59	2.00
747.61	748	0.59	2.00
807.04	807	0.59	2.00

Calibration Results : without adjustment

Photometric Accuracy

Wavelength (nm)	Certified Values of Reference Material (Abs)	UUC Reading (Abs)	Uncertainty of Measurement (±Abs)	Coverage Factor *k*
420.0	Zero	0.000	0.0028	2.00
	0.5750	0.573	0.0028	2.00
	0.7156	0.713	0.0028	2.00
	1.0176	1.014	0.0028	2.00
440.0	Zero	0.000	0.0028	2.00
	0.5598	0.557	0.0028	2.00
	0.7037	0.700	0.0028	2.00
	1.0013	0.997	0.0028	2.00
465.0	Zero	0.000	0.0028	2.00
	0.5222	0.522	0.0028	2.00
	0.6646	0.664	0.0028	2.00
	0.9444	0.945	0.0028	2.00
546.1	Zero	0.000	0.0028	2.00
	0.5234	0.523	0.0028	2.00
	0.7007	0.700	0.0028	2.00
	0.9992	0.999	0.0028	2.00
590.0	Zero	0.000	0.0028	2.00
	0.5573	0.556	0.0028	2.00
	0.7760	0.773	0.0028	2.00
	1.1104	1.108	0.0028	2.00
635.0	Zero	0.000	0.0028	2.00
	0.5648	0.565	0.0028	2.00
	0.7654	0.765	0.0028	2.00
	1.0961	1.096	0.0028	2.00

Remark

- Each individual filter is measured against the empty filter holder (blank) used to zero the spectrophotometer
- UUC = Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k* , providing a level of confidence of approximately 95 %.

-o0o-

Agilent Technologies

Agilent Technologies (Thailand) Limited
U CHU LIANG BLDG. 22/F UNIT A,D
968 RAMA 4 ROAD, SILOM, BANGRAK
Bangkok 10500 Thailand

Tel. +662 637 6363
Fax: +662 632 4334
Email: ccc-smt@agilent.com
Website: www.agilent.com/chem

Customer Contact:
ALS Laboratory Group (Thailand) Co Ltd Head Office

104 Phatthanakan 40 Phatthanakan Rd Khwaeng Phatthanakan Khet Suan

TAX ID : 0105540004859

chanattagarn.imchom@alsglobal.com
227158760

Invoice To:
ALS Laboratory Group (Thailand) Co Ltd Head Office

104 Phatthanakan 40 Phatthanakan Rd Khwaeng Phatthanakan Khet Suan

SERVICE REPORT

Customer Purchase Order Number:	**Customer Number:** 70371013
Service Request:	**Service Request Date:**
Service Order: 6006676060	**Service Confirmation:** 6905905441

REVIEW BY Tatthporn C.
APPROVED BY Sawita N.
NEXT CAL. DATE 7/4/2026

Delivery Site:
ALS Laboratory Group (Thailand) Co Ltd Head Office

104 Phatthanakan 40 Phatthanakan Rd Khwaeng Phatthanakan Khet Suan

Location:
Room
Bldg
Lab
Dept

Direct Inquiries to:
Contact Name: Customer Contact Center
Contact E-mail: ccc-smt@agilent.com
Contact Telephone: +662 637 6363
Contact Fax: +662 632 4334

products | applications | software | services

Learn more about Agilent's Special Offers, Products, Services and our full range of laboratory productivity solutions optimized for your applications and workflows. Visit us at www.agilent.com/chem

Service Confirmation Number: 6905905441

Service Confirmation Date: 08.10.2024

Service Instrument:

Model Number	Model Description	Serial Number	System Handle	Parent Asset
SYS-IM-7900	ICPMS 7900 System			
G8410A	SPS 4 Autosampler	AU15430722	ICP MS 7900	SYS-IM-7900
G8411A	ISIS 3 for Agilent 7850/7900/8900	JP15510227	ICP MS 7900	SYS-IM-7900
G3292A	PSC 6106T Chiller	2U15A1948	ICP MS 7900	SYS-IM-7900
G8403A	Agilent 7900 ICP-MS	JP15471169	ICP MS 7900	SYS-IM-7900

Service Items:

Item	Service/Part #	Description	Qty	Entitlement	Service Start	Service End
1000	EOQ	Enterprise Operational Qualification	1.00	Agreement Entitlement - 100 % covered	04.10.2024	04.10.2024
1010	5185-5850	ICP-MS Checkout Solutions	1.00	Agreement Entitlement - 100 % covered		

Additional Information:

Service Confirmation Number: 6905905441

Service Confirmation Date: 08.10.2024

Service Information:

Problem Description: *WU-EOQ-IM-7900-5001253655		
Service Provided: Perform OQ Hardware. Test CDS logon, auto sampler, Auto tune, BG and 20 Min stability. I calibrate the instrument No BKK_EL0043 test all pass.		
Service Overview Code: Reason Code: Scheduled Service Diagnosis Code: Scheduled Service Resolution Code: Scheduled Service		
Reported Hours: 7.0	**Travel Hours:** 2.0	
Customer Field Service Representative Name: **Panthep Kurasathain**	**Customer Field Service Representative Signature:**	**Date:** **08 Oct 2024**
Customer Name: **Supakwan Mak**	**Customer Signature:** Supakwan M.	**Date:** **08 Oct 2024**
Additional Comments:		

Metrological Center

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110

Telephone : +66 2 586 5792-4 Fax : +66 2 586 5109

Website : www.scieco.co.th E-Mail : calibrate@scg.co.th

Certificate No. T250355

Certificate of Calibration

Equipment	:	HEATING BLOCK
Manufacturer	:	Environmental Express
Model	:	SC 196
Serial No.	:	6974CECW3285
Customer Code	:	BKK_EL0054
ID No.	:	T5306A3
Customer	:	ALS Laboratory Group (Thailand) Co.,Ltd. 104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan, Khet Suan Luang, Bangkok 10250
Customer Location	:	Acid Digestion Lab
Date of Receipt	:	26 February 2025
Calibrated By	:	Atiphong Rongrat (Technician)
Approved By	:	_____ / Boonchai Suriyawong (Site Calibration Manager)
Date of Issue	:	17 MAR 2025

REVIEW BY Tattaporn C.

APPROVED BY Sawitn N.

NEXT CAL. DATE 04/09/25

The uncertainties are for a confidence probability of approximately 95%.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standard laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Metrological Center.

Metrological Center

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110

Telephone : +66 2 586 5792-4 Fax : +66 2 586 5109

Website : www.scieco.co.th E-Mail : calibrate@scg.co.th

Calibration Report

Equipment : **HEATING BLOCK**
Date of Calibration : **4 March 2025**
Environment : **Temperature : 24.4-24.9 °C**
Line Voltage : 221.6-226.3 V
Relative Humidity : 55 - 65 %RH

Condition of this results of calibration :

1. This equipment was calibrated by insert nine standard thermocouples type T into its chamber , the other one standard thermocouples type T use for ambient temperature measurement . The calibration was done in according to WI-T20.
   All data show below were final values and the initial data from customer request . The temperature scale used was based on ITS - 90 .
2. Reference Standard Instrument :

Instrument	Model	Instrument No.	Certificate No.	Due Date
TC	TYPE T	TN221-TN230	T240712	19 April 2025
TC	TYPE T	TN231-TN240	T240712	19 April 2025
TC	TYPE T	TN241-TN250	T240401	16 March 2025
TC	TYPE T	TN251-TN260	T240401	16 March 2025
DATA LOGGER	34970A	T193	T240401	16 March 2025

3. This certificate is traceable to :
   National Institute of Metrology (Thailand) through Metrological Center (NSC-TISI-TIS 17025 CALIBRATION 0244.)
4. Condition of calibrated item : good
   Equipment Description :
   Time Constant 2 Hour 40 Minute At 95 °C
   Fresh Air Damper ☐ Open ☐ Min ☐ Medium ☐ Max
   ☐ Close
   ☒ Not Available
5. Adjustment :
   ( ) without adjustment (X) after adjustment

Approved By.

Metrological Center

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110

Telephone : +66 2 586 5792-4 Fax : +66 2 586 5109

Website : www.scieco.co.th E-Mail : calibrate@scg.co.th

Calibration Report

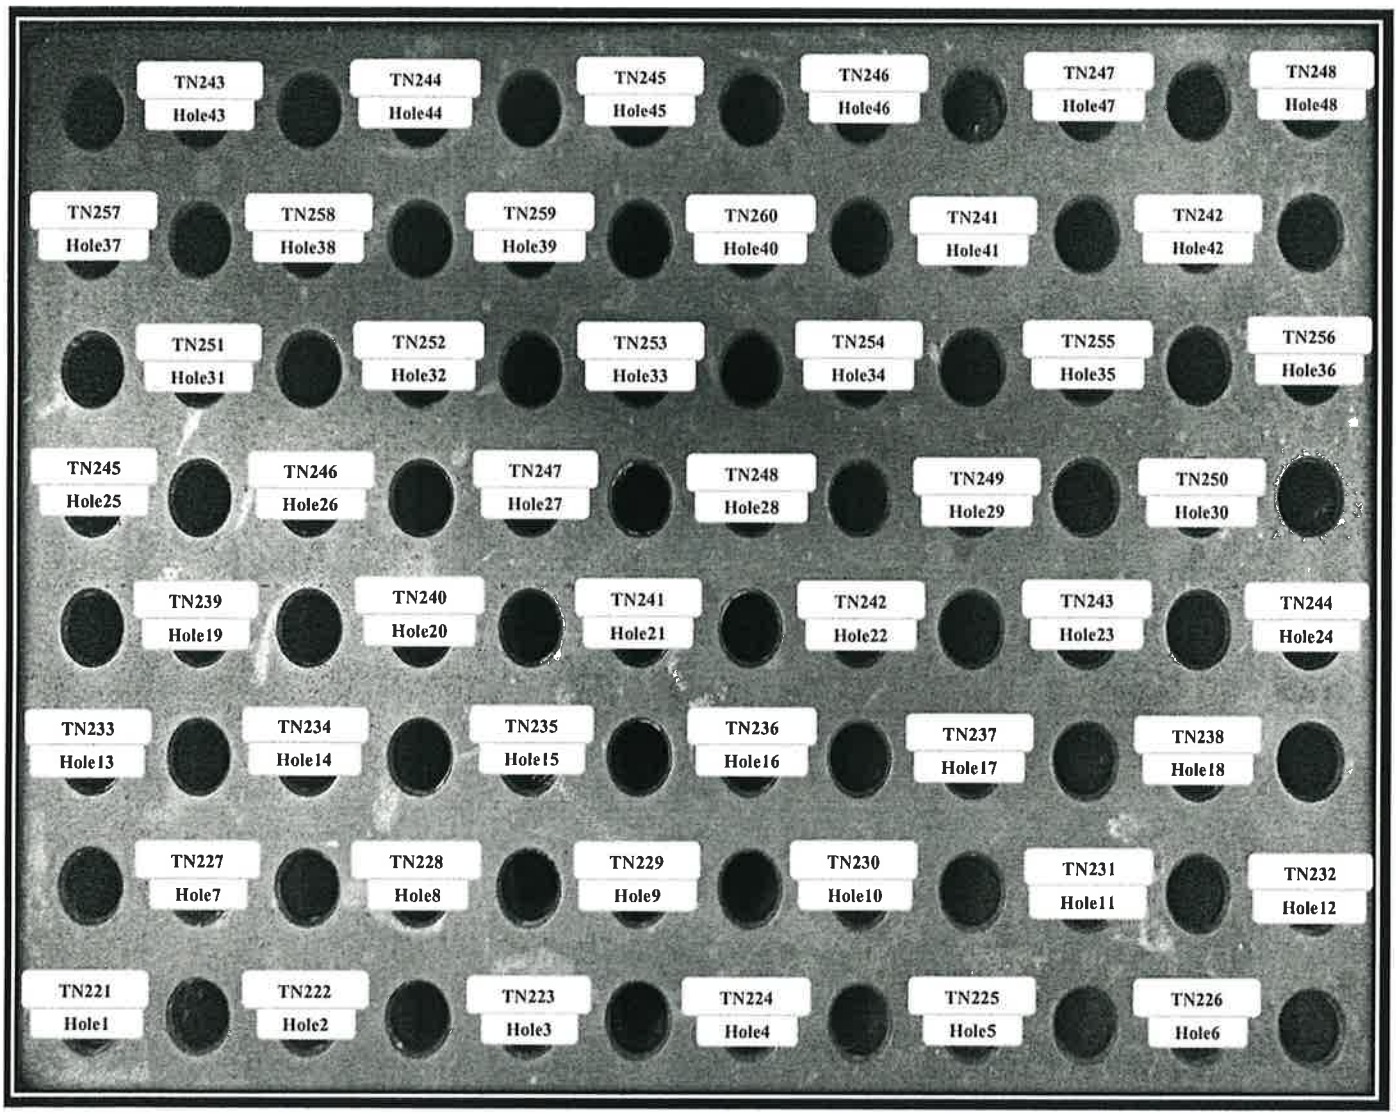

FRONT CONTROL

Approved By. _____

Metrological Center

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110

Telephone : +66 2 586 5792-4 Fax : +66 2 586 5109

Website : www.scieco.co.th E-Mail : calibrate@scg.co.th

Calibration Report

Measurement Results

Calibration Point		Average Standard Reading at each position (°C)					
R1 Hole1-Hole6		**TN221**	**TN222**	**TN223**	**TN224**	**TN225**	**TN226**
CAL POINT	Max	94.85	95.37	95.03	95.25	95.52	94.75
95	Min	94.17	94.66	94.38	94.63	94.87	94.12
	Average	94.51	95.02	94.70	94.94	95.20	94.43
R2 Hole7-Hole12		**TN227**	**TN228**	**TN229**	**TN230**	**TN231**	**TN232**
	Max	94.71	94.56	94.79	95.32	95.44	95.06
	Min	94.05	93.88	94.10	94.65	94.90	94.65
	Average	94.38	94.22	94.44	94.99	95.17	94.85
R3 Hole13-Hole18		**TN233**	**TN234**	**TN235**	**TN236**	**TN237**	**TN238**
	Max	95.26	95.43	95.40	95.71	95.41	95.06
	Min	94.54	94.64	94.71	95.10	94.86	94.42
	Average	94.90	95.03	95.06	95.41	95.13	94.74
R4 Hole19-Hole24		**TN239**	**TN240**	**TN241**	**TN242**	**TN243**	**TN244**
	Max	95.13	95.06	95.68	96.16	95.35	95.80
	Min	94.39	94.43	94.86	95.51	94.88	95.12
	Average	94.76	94.75	95.27	95.83	95.12	95.46
R5 Hole25-Hole30		**TN245**	**TN246**	**TN247**	**TN248**	**TN249**	**TN250**
	Max	94.95	95.81	95.39	95.82	95.66	95.66
	Min	94.47	95.03	94.67	94.99	94.84	94.87
	Average	94.71	95.42	95.03	95.41	95.25	95.27
R6 Hole31-Hole36		**TN251**	**TN252**	**TN253**	**TN254**	**TN255**	**TN256**
	Max	96.07	95.34	96.28	95.39	94.95	95.12
	Min	95.28	94.55	95.51	94.62	94.13	94.35
	Average	95.67	94.95	95.90	95.00	94.54	94.73
R7 Hole37-Hole42		**TN257**	**TN258**	**TN259**	**TN260**	**TN241**	**TN242**
	Max	95.15	95.63	96.11	95.09	95.34	95.51
	Min	94.38	94.88	95.32	94.28	94.54	94.72
	Average	94.76	95.25	95.71	94.69	94.94	95.11
R8 Hole43-Hole48		**TN243**	**TN244**	**TN245**	**TN246**	**TN247**	**TN248**
	Max	95.84	95.87	95.44	95.72	95.65	95.75
	Min	95.06	95.10	94.60	94.95	94.87	94.98
	Average	95.45	95.48	95.02	95.34	95.26	95.36

Approved By.

SCG
CEMENT-BUILDING MATERIALS

Metrological Center

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110

Telephone : +66 2 586 5792-4 Fax : +66 2 586 5109

Website : www.scieco.co.th E-Mail : calibrate@scg.co.th

Calibration Report

Measurement Results

Calibration Point		Average Standard Reading at each position (°C)					
R1 Hole1-Hole6		**TN221**	**TN222**	**TN223**	**TN224**	**TN225**	**TN226**
CAL POINT	Max	104.48	104.40	104.60	105.27	105.24	105.19
105	Min	104.15	104.02	104.25	104.94	104.91	104.93
	Average	104.32	104.21	104.42	105.10	105.08	105.06
R2 Hole7-Hole12		**TN227**	**TN228**	**TN229**	**TN230**	**TN231**	**TN232**
	Max	105.20	105.45	105.58	105.96	105.81	106.03
	Min	104.92	105.14	105.29	105.64	105.53	105.79
	Average	105.06	105.29	105.43	105.80	105.67	105.91
R3 Hole13-Hole18		**TN233**	**TN234**	**TN235**	**TN236**	**TN237**	**TN238**
	Max	106.09	106.14	105.83	106.25	105.97	105.88
	Min	105.80	105.89	105.57	106.00	105.69	105.65
	Average	105.94	106.01	105.70	106.13	105.83	105.77
R4 Hole19-Hole24		**TN239**	**TN240**	**TN241**	**TN242**	**TN243**	**TN244**
	Max	105.87	105.75	105.30	105.07	105.22	105.66
	Min	105.62	105.52	105.13	104.90	105.05	105.49
	Average	105.74	105.63	105.21	104.98	105.14	105.57
R5 Hole25-Hole30		**TN245**	**TN246**	**TN247**	**TN248**	**TN249**	**TN250**
	Max	105.62	105.54	105.52	105.75	105.97	105.69
	Min	105.45	105.35	105.31	105.57	105.81	105.49
	Average	105.53	105.44	105.41	105.66	105.89	105.59
R6 Hole31-Hole36		**TN251**	**TN252**	**TN253**	**TN254**	**TN255**	**TN256**
	Max	106.19	106.34	106.47	105.96	105.76	105.35
	Min	106.02	106.16	106.31	105.77	105.58	105.18
	Average	106.10	106.25	106.39	105.87	105.67	105.27
R7 Hole37-Hole42		**TN257**	**TN258**	**TN259**	**TN260**	**TN241**	**TN242**
	Max	106.21	105.59	105.45	105.36	106.08	106.09
	Min	106.04	105.42	105.28	105.20	105.90	105.92
	Average	106.12	105.51	105.37	105.28	105.99	106.00
R8 Hole43-Hole48		**TN243**	**TN244**	**TN245**	**TN246**	**TN247**	**TN248**
	Max	106.54	106.33	105.78	105.38	105.42	105.69
	Min	106.38	106.16	105.60	105.20	105.25	105.52
	Average	106.46	106.25	105.69	105.29	105.33	105.61

Approved By. _____

Metrological Center

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110

Telephone : +66 2 586 5792-4 Fax : +66 2 586 5109

Website : www.scieco.co.th E-Mail : calibrate@scg.co.th

Calibration Report

Measurement Results:

HEATING BLOCK			Temperature Distribution	
Setting (°C)	Reading (°C)		Stability (±°C)	Uncertainty (±°C)
	Min , Max	Average		
102.0	-	102.0	0.43	0.83
107.0	-	107.0	0.20	0.70

*** The quoted uncertainty exclude " uniformity "**

The calibration result apply only the above calibrated item.

The result of test was found accurate as shown on date and place of test only.

The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor *k* which for a t-distribution, providing a level of confidence of approximately 95 % .

Approved By. _____

SCG

Metrology Center

SCI ECO Services Company Limited

51 Moo 8, Tubkwang, Kaeng Khoi, Saraburi, Thailand 18260
Bangkok Tel : +668 9205 6851 , +669 81924 0059
Saraburi Tel : +669 8247 2360
Website : www.scieco.co.th E-Mail : calibrate@scg.co.th

NSC-TISI-TIS 17025
CALIBRATION 0244

Certificate No. T250873

Certificate of Calibration

Equipment	:	Chamber (Cooling Room)
Manufacturer	:	KOLDTECH
Model	:	KM 320
Serial No.	:	TBN-1012061/05
Customer Code	:	BKK_EN0167
ID No.	:	T2463A3
Customer	:	ALS Laboratory Group (Thailand) Co.,Ltd. 104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan, Khet Suan Luang, Bangkok 10250
Customer Location	:	Laboratory Room
Date of Receipt	:	28 May 2025
Calibrated By	:	Atiphong Rongrat (Technician)
Approved By	:	_____ / Boonchai Suriyawong (Site Calibration Manager)
Date of Issue	:	19 JUN 2025

REVIEW BY ..... Sirida K.

APPROVED BY ..... Siriluk P.

NEXT CAL DATE..... 04/12/26

The uncertainties are for a confidence probability of approximately 95%.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standard laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Metrological Center.

Certificate No. T250873

Calibration Report

Equipment : **Chamber (Cooling Room)**
Date of Calibration : **4 June 2025**
Environment : **Temperature : 23.4-24.9 °C**
Line Voltage : 221.4-230.2 V
Relative Humidity : 55 - 65 %RH

Condition of this results of calibration :

1. Thisequipment was calibrated by insert 16 standard thermocouples type T into its chamber , the other one standard thermocouples type T use for ambient temperature measurement . The calibration was done in according to WI-T20 (based on ASTM E145-94 (Reapproved 2001) and AS2853-1986).
   All data show below were final values and the initial data from customer request . The temperature scale used was based on ITS - 90 .
2. Reference Standard Instrument :

Instrument	Model	Instrument No.	Certificate No.	Due Date
TC	TYPE T	TN91-TN100	T242036	3 December 2025
TC	TYPE T	TN101-TN110	T242036	3 December 2025
DATA LOGGER	34970A	T121	T242036	3 December 2025

3. This certificate is traceable to :
   National Institute of Metrology (Thailand) through Metrological Center (NSC-TISI-TIS 17025 CALIBRATION 0244.)
4. Condition of calibrated item : good
   Equipment Description :
   Time Constant 2 Hour 20 Minute At 3 °C
   Fresh Air Damper ☐ Open ☐ Min ☐ Medium ☐ Max
   ☐ Close
   ☒ Not Available
5. Adjustment :
   (X) without adjustment ( ) after adjustment

Approved By. _____

Certificate No. T250873

Calibration Report

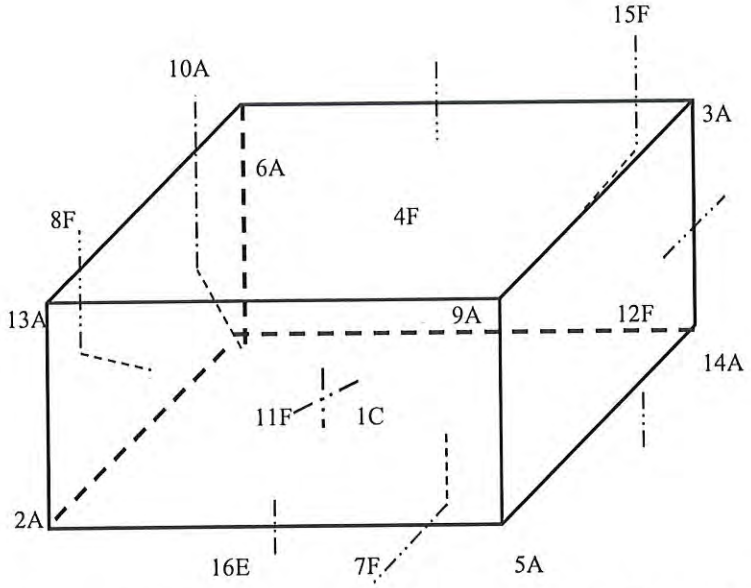

C = Centre , F = Centre of Face , A = Corner , E = Centre of Edge

1C	= TN91	
2A	= TN92	
3A	= TN93	
4F	= TN94	
5A	= TN95	
6A	= TN96	
7F	= TN97	
8F	= TN98	
9A	= TN99	
10A	= TN100	
11F	= TN101	

12F	= TN102
13A	= TN103
14A	= TN104
15F	= TN105
16E	= TN106

Approved By. _____

Certificate No. T250873

Calibration Report

Measurement Results

	Average Standard Reading at each position (°C)											
Calibration Point	TN91	TN92	TN93	TN94	TN95	TN96	TN97	TN98	TN99	TN100	TN101	TN102
3.0	2.95	2.92	3.09	2.92	3.16	3.50	3.40	3.03	3.14	2.98	3.44	3.13
	TN103	TN104	TN105	TN106								
	3.19	3.06	3.46	2.92								

Chamber (Cooling Room)			Temperature Distribution				
Setting (°C)	Reading (°C)		Average (°C)	Stability (±°C)	Uniformity (°C)	Uncertainty (±°C)	Coverage Factor *k*
	Min , Max	Average					
3.0	2.8 , 3.9	3.4	3.14	1.20	1.30	1.90	2.04

The calibration result apply only the above calibrated item.
The result of test was found accurate as shown on date and place of test only.
The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor *k* which for a t-distribution, providing a level of confidence of approximately 95 % .

Approved By._____

analytikjena
An Endress+Hauser Company

REVIEW BY Orawan T.
APPROVED BY Sawitr N.
NEXT CAL. DATE 12/06/2026

Maintenance Protocol

Atomic Fluorescence Spectrometer

mercur DUO / mercur DUO plus

analytikjena
An Endress+Hauser Company

Serial-No.: K170A0143 Customer-No.:

Date: 12 December 2024 Carried out by: Srichai Fak-on

Maintenance with following Operational Qualification (OQ) ☐
(requires a separate OQ protocol)

Company	บริษัท เอแอลเอส แลบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด
User	
Department	ห้องแลบปฏิบัติการ
Street	104 ซอย 40 ถนนพัฒนาการ แขวงสวนหลวง เขตสวนหลวง
Zip Code, City	กรุงเทพมหานคร 10250
Country	ประเทศไทย
Phone	
Fax	
E-mail	

Maintenance works basic unit

- [ ] tightness visual check inside the Mercur
- [ ] visual check if gold-traps are broken
- [ ] visual check if spectrometer is contaminated
- [ ] visual check of the fluorescence cell
- [ ] visual check of the absorption cell, incl. window
- [ ] reactor cleaning
- [ ] check pump-hose, if necessary change it
- [ ] check swivel drive (SEV)
- [ ] check drying-hose, output gas-liquid-separator
- [ ] test Bubble-Sensor
- [ ] check gas flows
- [ ] check volume flows, reagents
- [ ] recording stray light values
- [ ] measurement with 30 ng/l

Maintenance works Autosampler

Serial No.: 701 739

- [ ] lubricate the dosing-winding (Teflon-grease-spray)
- [ ] clean the dosing cylinder, if necessary exchange it
- [ ] lubricate the winding system of the height drive with some drops of oil
- [ ] check the toothed belt
- [ ] check the position of the mechanical stopper (height: 13mm)
- [ ] check the pump rate of mixing pump (<14s AS52, typ.7s/<20s AS52S, typ.10s)
- [ ] check the pump rate of washing cup
- [ ] check the electrical hose connections for good contact
- [ ] check the connectors of the magnetic valves
- [ ] check the dosing hose for buckling, if necessary exchange it

Device parameter		nominal value	actual value
visual check general tightness inside the Mercur		o.k.: ☑	changed: ☐
visual check Goldtraps		o.k.: ☑	changed: ☐
visual check spectrometer			
	Fluorescence cell	o.k.: ☑	changed: ☐
	Absorption cell, incl. window	o.k.: ☑	changed: ☐
	lens	o.k.: ☑	changed: ☐
	Swivel drive (SEV)	o.k.: ☑	changed: ☐
check pump hoses		o.k.: ☑	changed: ☐
check hoses and hose connectors		o.k.: ☑	changed: ☐
check and clean reactor		o.k.: ☑	changed: ☐
check drying hose output Gas-liquid-seperator		o.k.: ☑	changed: ☐
check bubble-sensor		o.k.: ☑	not o.k.: ☐
Check gasflow			
	Argon pressure valve 4	1.2 – 1.5 bar	1.5 bar
	Valve 1	10 Nl/h or 0.166 NL/min	0.142 NL/min
	Valve 2	50 Nl/h or 0.833 NL/min	0.785 NL/min
	Valve 3	5 Nl/h or 0.083 NL/min	0.080 NL/min
	Valve 4	10 Nl/h or 0.166 NL/min	-
Check liquidflow			
	Acid	2.5ml/min ± 1 ml	2.5 ml/min
	Red.-agent	2.5ml/min ± 1 ml	2.5 ml/min
	Sample	10ml/min ± 2 ml	10 ml/min
Adventitious light - values	**(V)**	**from file**	
	100	0	0
	200	0	0
	300	0	0
	350	0	0
	400	1	1
	450	2	3
	500	6	7
	550	13	15
	575	18	21
	600	25	29

Device parameter	nominal value	actual value
Analytical parameters Fluorescence cell		
Conditions.: max.conc.: 10µg/L PMT-voltage: .....360.....V		
Blank-solution		Int ...0.00044...
without enrichment / FBR 30 ng/L	Int > 0.0015 RSD < 3 %	Int_1...0.00237... RSD...1.30...%
Conditions.: max.conc.: 1.7µg/L PMT-voltage: .....352.....V		
Blank-solution		Int.....–.....
with enrichment / FBR 30 ng/L	Int > 0.008 RSD < 3 %	Int_2.....–..... RSD.....–.....%
Fok.- factor (Int_2 / Int_1)	> 3.5	–
Analytical parameters Absorption cell		
Blank-solution		Ext...0.0011...
without enrichment / FBR 100 ng/L	Ext. > 0.0012 RSD < 5 %	Ext...0.0039... RSD..2.99...%
Comments		
• การใช้งานของ Tech: With enrichment ไม่สามารถวัดค่าได้เนื่องจาก Valve 4 (Gas flow) ไม่ทำงาน แต่เช็คแรงดันไฟจาก Board control จ่ายปกติ 24 Vdc. • หากมีตัวอย่างที่ต้องวัดด้วย Tech: With enrichment ต้องซ่อมเปลี่ยนตัว Gas box		

Signature Technician

12 December 2024

Place, Date (DD/MM/YYYY)

Signature Customer

12 December 2024

Place, Date (DD/MM/YYYY)

analytikjena
An Endress+Hauser Company

35 Moo 5. 345 Road, Khlong Khoi, Pak Kret,
Nonthaburi. 11120 Thailand.
Phone: +66(2) 1062970-72
Fax: +66(2) 1062973
www.analytik-jena.com

Service Report

Customer's address :	Customer's Ref. No. Co no. Service 2024
บริษัท เอแอลเอส แลบอราทอรี่ กรุ๊ป (ประเทศไทย) จำกัด	
104 ซอย 40 ถนนพัฒนาการ แขวงสวนหลวง เขตสวนหลวง กรุงเทพมหานคร 10250	
E-mail :	Phone : Fax :

☑ Analytik Jena Instruments (Thailand) Ltd.
☐ Analytik Jena Far East (Thailand) Ltd.

Job No. 2412571PB	User :	Service Engineer : ศรีชัย ฟักอ่อน	Date : 12/12/2024	Page : 1/1
Instrument model : Mercury	Serial No. K170A0143		Software Version No. WinAAS 4.7.9.0	

☐ Repair (RE) ☑ Maintenance (PM) ☐ Installation (IN) ☐ Warranty ☐ Application (AP) ☐ Site Prep.(SP) ☐ Visit(VI)

Fault / Claim : เข้าทำ PM เครื่อง Mercury (Contactyear 2025 / 1 Time) ☐☐☐ Error Code

Action taken :

- Maintenance work basic unit
- Check Device parameters
- Check gas flow
- Check liquid flow
- Check Adventitious light- Valves
- Test run Analytical parameter Fluorescence cell
- Test run Analytical parameter Absorption cell

Hg Valve ทำไม่ได้ครับ
อุปกรณ์ในไฟลากต่อ Board ที่ 24 V ปกติ

Action Pending / Recommendation :

- เครื่องปกติในโหมดของ Tech: Without enrichment และ Hg absorption
- Hg low pressure lamp (Energy ต่ำต้องปรับค่า PMT voltage สูง) แนะนำให้เปลี่ยนอะไหล่ชุด Hg low pressure lamp

เปลี่ยนชุด Consumable ของปีถัดไปนี้ไว้ด้วย

☐ Spare Part ☑ Instrument Configuration :

Item No.	Name	Quantity	Unit Price
1. 403.325	5-Valve assembly (SMC / Gas box)	1	
2. 407-401.502	Hg low pressure lamp	1	
3.			
4.			
5.			
6.			
7.			
8.			

Herewith the undersigned confirm the time devoted, the work performed, the perfect function of the device, and the receipt/delivery of the specified spare parts. *Traveled hours and kilometers can only be entered after the return of the service engineer.	Date / Signature of Customer	Date / Signature of Service Engineer	Work completed?
	Orawan T.		☑ Yes ☐ No

Services are subject to the General Terms and Conditions of Analytik Jena AG, which will be sent on request.

Mercur

Report file:	C:\WinAAS\TMP\2024\Dec\Pro_008		
Program version:	4.7.10.0	Printed on:	12/12/2024 11:37
		Recording started on	12/12/2024 11:27 GMT+7.0
Operator:	PSU,OTA		
Laboratory:	ALS-BKK		
Code:	II_Hg067_2024		

Remarks:

Food,water

Method parameters

Hg

Method	Without enrichment / FBR 30ng/L_PM24052023
Created on	5/24/2023 Time 12:27
Program	---

Parameters Mercur Technique: Hg fluorescence

Line	253.7 nm		
Lamp type	Hg-LP		
Integr. mode	Peak height	Integr. time	30 s
PMT	360 V		
AZ time	5 s	Peak smoothing	12/11
Delay	0 s		

Working mode	w/o enrich.	System cleaning	Acid
FBR technique	on	Wash time acid	10 s
Pump speed	3	Soaking time	20 s
Sample load time	10 s	Gas load time	5 NL/h
Reaction time	10 s		
Waiting time AZ	5 s		
Delay	0 s		
Purge time1	28 s		
Purge time2	15 s	Gas wash time2	10 NL/h

Autosampler

Autosampler	AS51S/F	Tray type	87/139
Working mode	continuous		
Dilution	---		

QC parameters

QC type	Conc. check		
QC check samp. 1	---	QC check samp. 2	---
Conc.	---	Conc.	---
Error limit	---	Error limit	---
Rep. measurement	off	Reaction	flag + continue
QC std.1 no.	1(30.000 ng/L)	QC std.2 no.	1(30.000 ng/L)
QC std.1 limit	± 50.00%	QC std.2 limit	± 50.00%
QC std. act.	flag + continue		
Expect. blank abs.	0.0100± 0.0100	Reaction	flag + continue
QC precision	off		
		Reaction	off
		QC Recal.factor	Off

Calibration settings

Calib. meth	Standard calib.	Calibr. unit	ng/L
No. standards	1	Conversion fac.	1000000
Type of standards	---	Standard prep.	Premixed
		Blank correct.	---
		Recalib. std. no.	---
Output unit	µg/L	Conversion fac.	1000
Calib. stat.	Mean	Meas. cycles	3
		Blind cycles	1
Stock sol. 1	---	Stock sol. 2	---
Stock sol. 3	---	Stock sol. 4	---
Type of cal. curve	linear	Intercept	calculated
Weighted cal.	off	Grubbs stat.	off
Check of cal. curve	no outlier test		

Sample statistics

Stat. mode	Mean	Meas. cycles	2
Confid. level	95.4 %	Blind cycles	1
Grubbs stat.	---		

Calibration standards **Hg**

No	Name	State	Pos	Conc./ ng/L	Ints	SD	RSD/%
1	Cal-Zero	(--)	79	0.000	H: **0.000445**	**0.000017**	**3.813**
					A: 0.009414	0.000140	1.497
2	Cal-Std1	(--)	80	30.000	H: **0.002375**	**0.000031**	**1.306**
					A: 0.03403	0.000423	1.244

Calibration function 1 **12/12/2024 11:36 Calibration (Peak height)**

Ints=k1+k2*conc

k1=0.000446 k2=0.000064 Recal. factor: ---

Slope	0.00006 Ints/(ng/L)	R2-adjusted	1.0000
sc0	1.00000 ng/L		
Lower limit	0 ng/L	Upper limit	33.0 ng/L
Detection limit	---	Deter. limit	---

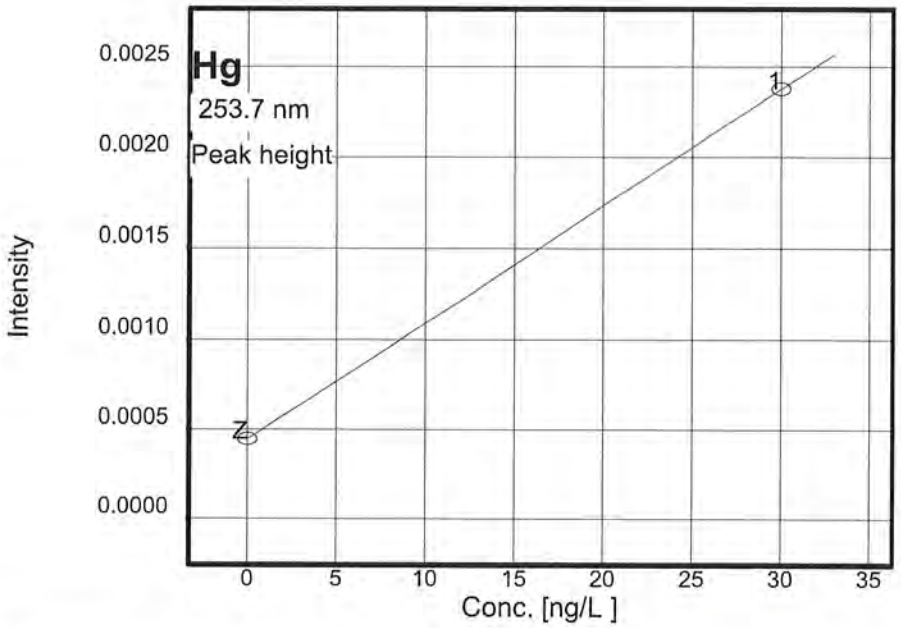

Measurements and events (sorted by time)

Hg	Without enrichment / FBR 30ng/L_PM 24052023					12/12/2024	11:28
ID	**Conc.**	**Ints**	**BG**	**SD**	**RSD/%**	**Int. type**	**Time**
Cal-Zero		0.000436				PkH	11:30
		0.000436					11:31
		0.000465					11:32
	0ng/L	0.000445		0.000017000	3.813		11:32
Cal-Std1		0.002402				PkH	11:34
		0.002341					11:35
		0.002381					11:36
	30.00ng/L	0.002375		0.000031020	1.306		11:36
Calibration	Calibration function: 01						11:36

Peak plots **Hg**

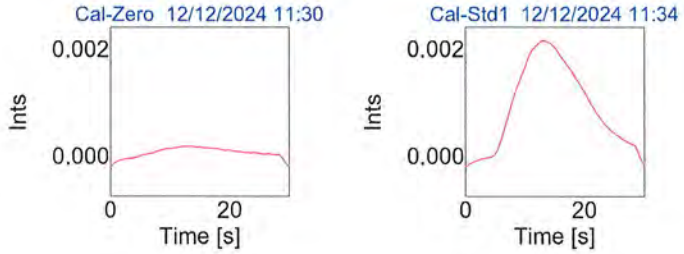

Mercur

Report file:	C:\WinAAS\TMP\2024\Dec\Pro_010		
Program version:	4.7.10.0	Printed on:	12/12/2024 13:31
		Recording started on	12/12/2024 13:16 GMT+7.0
Operator:	PSU,OTA		
Laboratory:	ALS-BKK		
Code:	II_Hg067_2024		

Remarks:

Food,water

Method parameters

Hg

Method	Without enrichment / Abs / FBR 100ng/L_PM 24052023
Created on	12/12/2024 Time 12:42
Program	---

Parameters Mercur Technique: Hg absorption

Line	253.7 nm		
Lamp type	Hg-LP		
Integr. mode	Peak height	Integr. time	55 s
PMT	225 V		
AZ time	5 s	Peak smoothing	8/5
Delay	8 s		

Working mode	w/o enrich.	System cleaning	Acid
FBR technique	on	Wash time acid	15 s
Pump speed	4	Soaking time	20 s
Sample load time	8 s	Gas load time	5 NL/h
Reaction time	12 s		
Waiting time AZ	15 s		
Delay	10 s		
Purge time1	50 s		
Purge time2	10 s	Gas wash time2	10 NL/h

Autosampler

Autosampler	AS51S/F	Tray type	87/139
Working mode	continuous		
Dilution	---		

QC parameters

QC type	Conc. check		
QC check samp. 1	---	QC check samp. 2	---
Conc.	---	Conc.	---
Error limit	---	Error limit	---
Rep. measurement	off	Reaction	flag + continue
QC std.1 no.	1(100.00 ng/L)	QC std.2 no.	1(100.00 ng/L)
QC std.1 limit	± 50.00%	QC std.2 limit	± 0.00%
QC std. act.	flag + continue		
Expect. blank abs.	0.0100± 0.0100	Reaction	flag + continue
QC precision	off		
		Reaction	off
		QC Recal.factor	Off

Calibration settings

Calib. meth	Standard calib.	Calibr. unit	ng/L
No. standards	1	Conversion fac.	1000000
Type of standards	---	Standard prep.	Premixed
		Blank correct.	---
		Recalib. std. no.	---
Output unit	µg/L	Conversion fac.	1000
Calib. stat.	Mean	Meas. cycles	3
		Blind cycles	1
Stock sol. 1	---	Stock sol. 2	---
Stock sol. 3	---	Stock sol. 4	---
Type of cal. curve	linear	Intercept	calculated
Weighted cal.	off	Grubbs stat.	off
Check of cal. curve	no outlier test		

Sample statistics

Stat. mode	Mean	Meas. cycles	2
Confid. level	95.4 %	Blind cycles	1
Grubbs stat.	---		

Calibration standards **Hg**

No	Name	State	Pos	Conc./ ng/L	Abs	SD	RSD/%
1	Cal-Zero	(--)	79	0.00	H: **0.001129** A: 0.039764	**0.000086** 0.004386	**7.666** 11.03
2	Cal-Std1	(--)	81	100.00	H: **0.003950** A: 0.070560	**0.000118** 0.004290	**2.993** 6.081

Calibration function 1 **12/12/2024 13:31 Calibration (Peak height)**

Abs=k1+k2*conc

k1=0.001130 k2=0.000028 Recal. factor: ---

Slope	0.00003 Abs/(ng/L)	R2-adjusted	1.0000
sc0	1.00000 ng/L	Charact. conc.	154.568 (ng/L)/1%I
Lower limit	0 ng/L	Upper limit	110. ng/L
Detection limit	---	Deter. limit	---

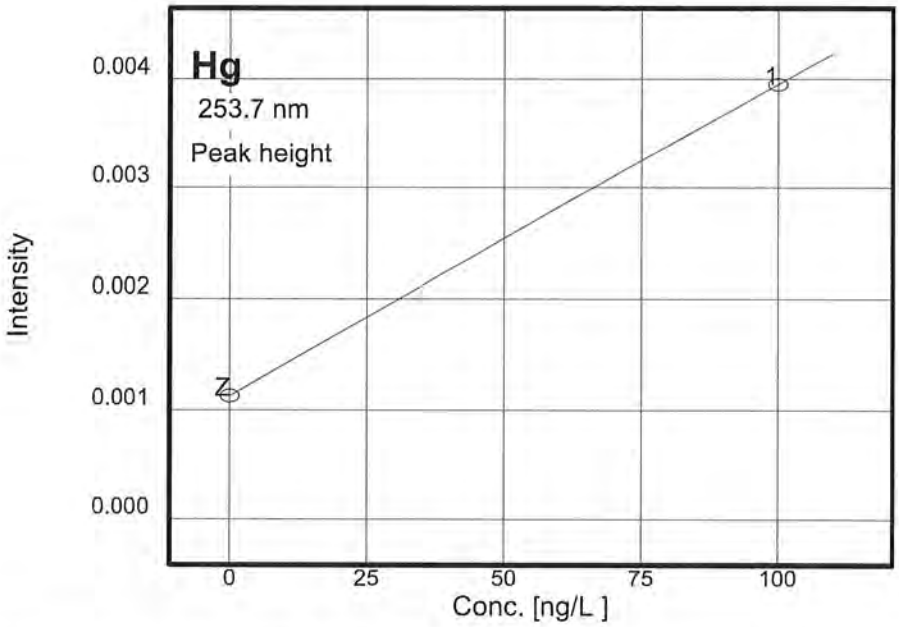

Measurements and events (sorted by time)

Hg	Without enrichment / Abs / FBR 100ng/L_PM 24052023					12/12/2024	13:16
ID	**Conc.**	**Abs**	**BG**	**SD**	**RSD/%**	**Int. type**	**Time**
Cal-Zero		0.001062				PkH	13:19
		0.001227					13:20
		0.001099					13:22
	0ng/L	0.001129		0.000086605	7.666		13:22
Cal-Std1		0.003949				PkH	13:26
		0.004069					13:27
		0.003832					13:29
	100.ng/L	0.003950		0.00011825	2.993		13:29
Calibration	Calibration function: 01						13:31

Peak plots **Hg**

Automation Service Co.,Ltd.

Head Office : 929,929/1 Soi Pattanakarn 30, Pattanakarn Road, Suanluang, Bangkok
Tel: 02-319-9994
www.automation.co.th

Sales & Service Center
Rayong : 1/15 Huaypong Rd., Muang, Rayong 21150 [T. 038-692-152]
Lamphun : 122/5 M.4, Ban Klang, Muang, Lamphun 51000 [T. 053-581-876]
Prachinburi : 688 M.10, Thatum, Srimahaphote, Prachinburi 25140 [T. 037-208-880]

BKK_EN0066

MTOC : L-0617/2025

Report No. : ALS-416

TOC-L Maintenance Report

Instrument	: Total Organic Carbon Analyzer	Measuring	: TC 0 ~ 30000 mg/L
Model	: TOC-LCSH	Place of Installation	: -
Serial No.	: H54425300416	Department	: LABORATORY
Manufacture	: Shimadzu		

Customer

ALS Laboratory Group (Thailand) Co.,Ltd.
104 Phatthanakan 40, Phatthanakan Rd.,
Khwaen Suan Luang, Khet Suan Luang,
Bangkok 10250 Thailand

Date of Maintenance : 27 / 06 / 2025

REVIEW BY Uban S.
APPROVED BY Sirilut B.
NEXT CAL. DATE 27/6/26

Ambient Condition : Temperature 25.5 ± 5 °C

: Humidifier 58 ± 15 %RH

Maintenance By : Teeraphat Kamlungkua

(Mr. Teeraphat Kamlungkua)
Technician

Approved By :

(Mr. Nipon Phungsomsak)
Technician Manager

User Name : Sirilut B.

(Miss Sirilut Bunnak)

Automation Service Co.,Ltd.

Head Office : 929,929/1 Soi Pattanakarn 30, Pattanakarn Road, Suanluang, Bangkok
Tel: 02-319-9994
www.automation.co.th

Sales & Service Center
Rayong : 1/15 Huaypong Rd., Muang, Rayong 21150 [T. 038-692-152]
Lamphun : 122/5 M.4, Ban Klang, Muang, Lamphun 51000 [T. 053-581-876]
Prachinburi : 688 M.10, Thatum, Srimahaphote, Prachinburi 25140 [T. 037-208-880]

MTOC : L-0617/2025

Report No. : ALS-416

Maintenance Sheet

Customer : ALS Laboratory

Date : 27 / 06 / 2025

Model : TOC-LCSH

Serial No. H54425300416

Item	Carry out maintenance work	Result	Exchange	Comment
1.	Check functionality of the device			
	Check furnace temperature (Standard cat. 680 °C / for TN cat. 720 °C)	O.K.		
	Check dehumidifier temperature (1 °C)	O.K.		
	Check the entire flow line related to leakage	O.K.		
	Check baseline status (OK)	O.K.		
	Check carrier gas pressure (200 ±10 kPa)	O.K.		
	Check carrier gas flow rate (150 mL/min)	O.K.		
2.	Tubes			
	Check all tubing for contamination, if necessary clean them	O.K.		
	Check all tubing for tight connection	O.K.		
3.	Container and Drainage			
	Fill up humidifier with pure water to max. level	O.K.		
	Check filling of dilution water and acid container	O.K.		
	Rinse Drain Pot, after wards refill again with pure water	O.K.		
	Check if outlet flow is in proper conditions	O.K.		
4.	TC and IC Injection			
	Clean injector Block	O.K.		
	Check injector Block for wear	O.K.		
	Check injection tube adjustment	O.K.		
	Check injection for leakage	O.K.		
	Check injection for clogging	O.K.		
5.	IC Measurement (N-type)			
	Check acidification in syringe			
	Check sparging in syringe			
6.	Eye check of 8-Port valve, for sample residues or moist spots that indicate possible leakage	O.K.		
7.	Check and if necessary exchange consumable, Maintenance parts	O.K.		See list of consumable, maintenance parts

Inspection by : Teeraphat Kamlungkua

(Mr. Teeraphat Kamlungkua)
Technician

SHIMADZU ANALYZER

Automation Service Co.,Ltd.
Head Office : 929,929/1 Soi Pattanakarn 30, Pattanakarn Road, Suanluang, Bangkok
Tel: 02-319-9994
www.automation.co.th

Sales & Service Center
Rayong : 1/15 Huaypong Rd., Muang, Rayong 21150 [T. 038-692-152]
Lamphun : 122/5 M.4, Ban Klang, Muang, Lamphun 51000 [T. 053-581-876]
Prachinburi : 688 M.10, Thatum, Srimahaphote, Prachinburi 25140 [T. 037-208-880]

MTOC : L-0617/2025 Report No. : ALS-416

Item	Carry out maintenance work	Result	Exchange	Comment
8.	Due to instrument condition, clean the instrument inside and outside.	O.K.		
9.	After checking the system and exchanging of consumable and maintenance parts a new 1-3 point calibration have to be done.	O.K.		Addition test 1.
10.	After wards the calibration perform check sample measurement.	O.K.		Addition test 2.

Addition test

Test no.	Test conditions	Meas. value	Result
1.	Calibration TC standard solution at 0, 0.1, 0.5, 1, 5 10, 20 injection volume 50 µL No. of measurement 2 times (Max.3)		Attachment : ALS-416 Page 1/4 -2/4
	Criteria : R^2 = 0.995 or more	0.9999	Pass
2.	Measurement of reagent water and TC standard solution at 5.0 mg/L injection volume 50 µL No. of measurement 2 times (Max.3) and calculate accuracy by Meas. of TC standard – Meas. of Reagent water		Attachment : ALS-416 Page 3/4 - 4/4
	Criteria : Accuracy %Recovery 10% or less	5.244 – 0.1797 = 5.064 ppm	Pass

Inspection by : Teeraphat Kamlungkua

(Mr. Teeraphat Kamlungkua)
Technician

Automation Service Co.,Ltd.

Head Office : 929,929/1 Soi Pattanakarn 30, Pattanakarn Road, Suanluang, Bangkok
Tel: 02-319-9994
www.automation.co.th

Sales & Service Center
Rayong : 1/15 Huaypong Rd., Muang, Rayong 21150 [T. 038-692-152]
Lamphun : 122/5 M.4, Ban Klang, Muang, Lamphun 51000 [T. 053-581-876]
Prachinburi : 688 M.10, Thatum, Srimahaphote, Prachinburi 25140 [T. 037-208-880]

MTOC : L-0617/2025

Report No. : ALS-416

List of Consumable, Maintenance parts

Pos.	Part Number	Part Name	Result	Exchange	Recommended Interval
1.	036-11209-84	O-ring, 4D P10A (Viton , for TC,IC Slider)	O.K.		1 time per year, Depending on condition
2.	036-11219-84	O-ring, 4D P20 (for sealing TC-Combustion tube)	O.K.	√	1 time per year, Depending on condition
3.	638-15025	O-ring, PIFE (for TC,IC-Slider)	O.K.		1 time per year, Depending on condition
4.	630-00105-01	Platinum net, (2pcs-set) (to support catalyst)	O.K.	√	6 month same time as catalyst exchange
5.	630-00557	Silica Wool (to support catalyst)	O.K.	√	6 month same time as catalyst exchange
6.	630-00992	Halogen Scrubber	O.K.	√	6 month
7.	630-00996	High Sensitivity TC Catalyst (When installed)	N/A		Depending on condition
8.	638-60116	Regular Catalyst (33g) (When installed)	O.K.	√	6 month
9.	638-56251-01	8-Port valve rotor	O.K.	√	1 time per year
10.	638-41323	TC-Combustion Tube	O.K.	√	6 month same time as catalyst exchange
11.	631-43404-01	Packing, gasket slider (for TC-Injection tube)	O.K.		1 time per year, Depending on condition
12.	638-59296	Syringe 5mL	O.K.		Depending on condition
13.	638-59296-01	Plunger Tip (for syringe 5mL)	O.K.	√	6 month
14.	042-00405-11	IC reagent supply pump head	O.K.		1 time per year
15.	630-00999	CO2-Absorber (for cell space purge)	O.K.	√	1 time per year
16	630-00964	Molecular Sieves 13x	O.K.		1 time per year

Note. Table indicates the guidelines replacement periods when NPOC measurement is performed on sample that are comparatively as clean as tap water ,use standard catalyst and at a rate of about 500 sample per month (operating five days a week)

Inspector By Teeraphat Kamlungkua

(Mr. Teeraphat Kamlungkua)
Technician

TOC-Control L Report

ALS
2025_06_27_001_PM.tlx

Instr.Information

Instrument Options	TOC/ASI/IC Unit/
Catalyst	Regular Sensitivity

Cal. Curve

Sample Name:	Untitled
Sample ID:	Untitled
Cal. Curve:	TC 0.1 - 20 ppm.2025_06_27_13_27_34.cal
Status	Completed

Type	Anal.
Standard	TC

Conc: 0.000mg/L

No.	Area	Inj. Vol.	Aut. Dil.	Rem.	Ex.	Date / Time
1	0.3995	50uL	1.000	*******		6/27/2025 1:30:33 PM
2	0.3474	50uL	1.000	*******		6/27/2025 1:32:43 PM

Acid Add.	0.000%
Mean Area	0.3735
SD Area	0.03684
CV Area	9.86%

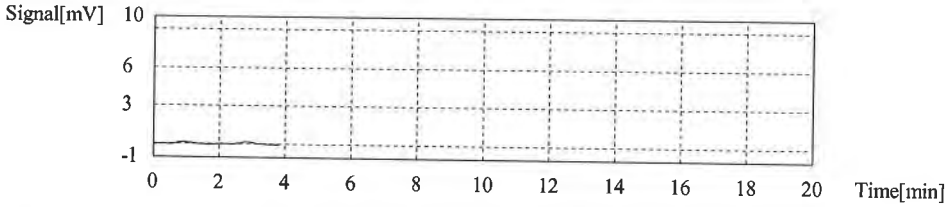

Conc: 0.1000mg/L

No.	Area	Inj. Vol.	Aut. Dil.	Rem.	Ex.	Date / Time
1	0.8247	50uL	10.00	*******		6/27/2025 1:39:33 PM
2	0.8513	50uL	10.00	*******		6/27/2025 1:42:22 PM

Acid Add.	0.000%
Mean Area	0.8380
SD Area	0.01881
CV Area	2.24%

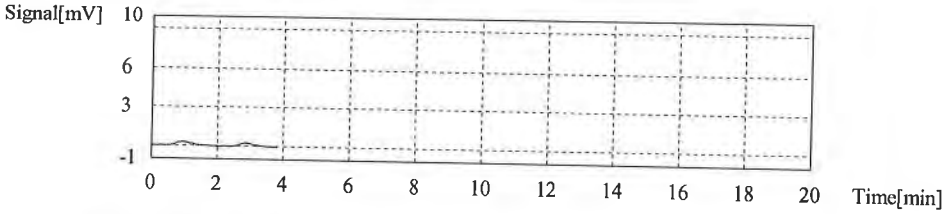

Conc: 0.5000mg/L

No.	Area	Inj. Vol.	Aut. Dil.	Rem.	Ex.	Date / Time
1	2.097	50uL	2.000	*******		6/27/2025 1:48:37 PM
2	2.304	50uL	2.000	*******	E	6/27/2025 1:50:49 PM
3	1.893	50uL	2.000	*******	E	6/27/2025 1:52:58 PM
4	2.014	50uL	2.000	*******		6/27/2025 1:55:07 PM

Acid Add.	0.000%
Mean Area	2.056
SD Area	0.05869
CV Area	2.86%

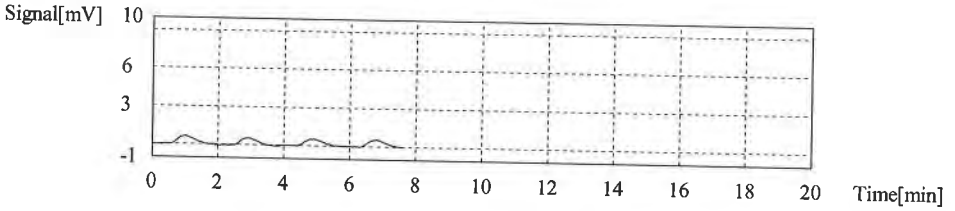

Conc: 1.000mg/L

TOC-Control L Report

ALS
2025_06_27_001_PM.tlx

No.	Area	Inj. Vol.	Aut. Dil.	Rem.	Ex.	Date / Time
1	3.357	50uL	1.000	*******	E	6/27/2025 1:58:14 PM
2	3.505	50uL	1.000	*******		6/27/2025 2:00:24 PM
3	3.501	50uL	1.000	*******		6/27/2025 2:02:36 PM

Acid Add. 0.000%
Mean Area 3.503
SD Area 0.00283
CV Area 0.08%

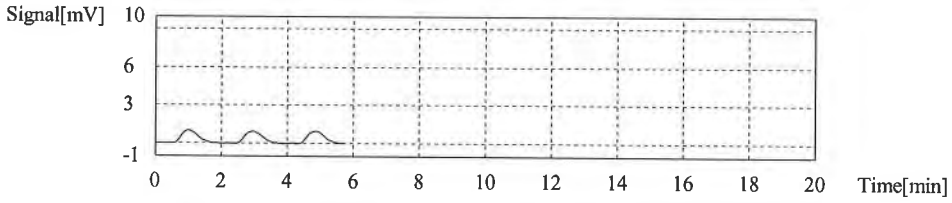

Conc: 5.000mg/L

No.	Area	Inj. Vol.	Aut. Dil.	Rem.	Ex.	Date / Time
1	14.19	50uL	4.000	*******		6/27/2025 2:09:44 PM
2	14.45	50uL	4.000	*******		6/27/2025 2:12:35 PM

Acid Add. 0.000%
Mean Area 14.32
SD Area 0.1838
CV Area 1.28%

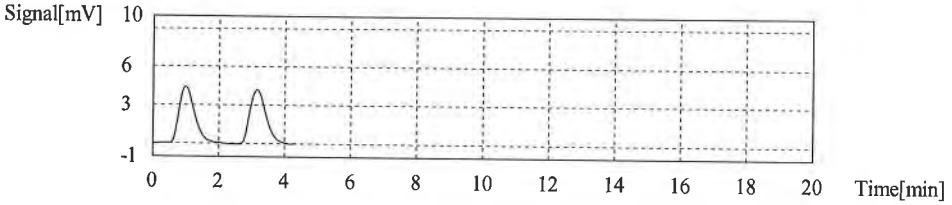

Conc: 10.00mg/L

No.	Area	Inj. Vol.	Aut. Dil.	Rem.	Ex.	Date / Time
1	28.15	50uL	2.000	*******		6/27/2025 2:19:03 PM
2	28.36	50uL	2.000	*******		6/27/2025 2:21:37 PM

Acid Add. 0.000%
Mean Area 28.26
SD Area 0.1485
CV Area 0.53%

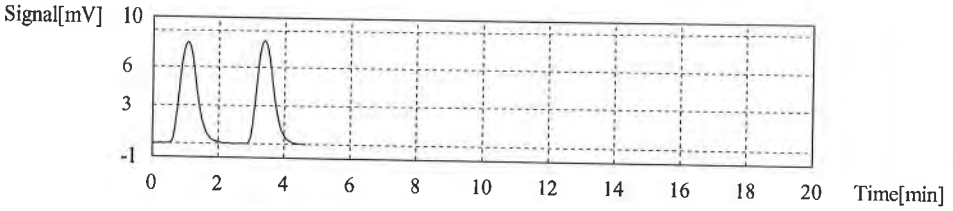

Conc: 20.00mg/L

No.	Area	Inj. Vol.	Aut. Dil.	Rem.	Ex.	Date / Time
1	55.05	50uL	1.000	*******		6/27/2025 2:25:14 PM
2	54.69	50uL	1.000	*******		6/27/2025 2:27:50 PM

Acid Add. 0.000%
Mean Area 54.87
SD Area 0.2546
CV Area 0.46%

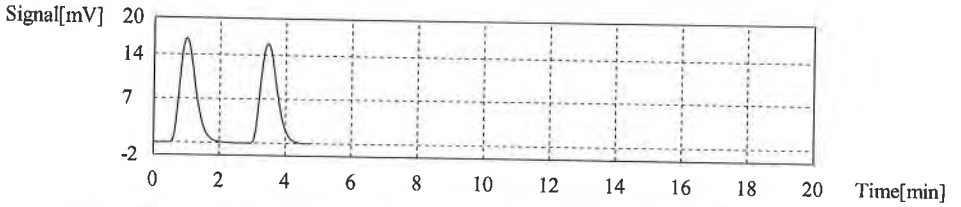

Slope: 2.721
Intercept 0.000
r^2 0.9999
r 0.9999
RSE(%) N/A
Zero Shift Yes

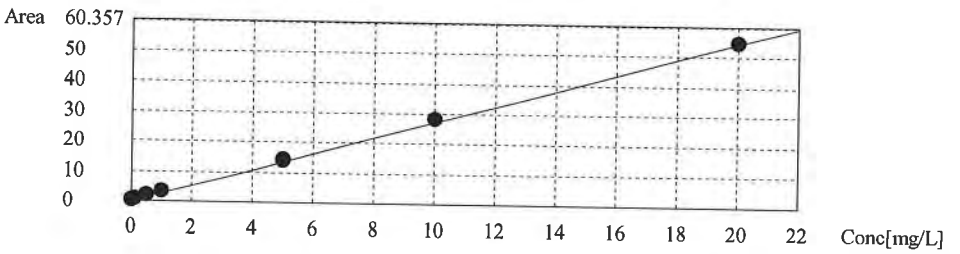

TOC-Control L Report

ALS
2025_06_27_001_PM.tlx

Instr.Information

Instrument Options	TOC/ASI/IC Unit/
Catalyst	Regular Sensitivity

Sample

Sample Name:	water
Sample ID:	Untitled
Origin:	TC 0.1 - 20 ppm.cal
Status	Completed
Chk. Result	

Type	Anal.	Manual Dilution	Result
Unknown	TC	1.000	TC:0.1797mg/L

1. Det

Anal.: TC

No.	Area	Conc.	Inj. Vol.	Aut. Dil.	Ex.	Cal. Curve	Date / Time
1	0.5210	0.1915mg/L	50uL	1.000		TC 0.1 - 20 ppm.2025_06_27_13_27_34.cal	6/27/2025 2:30:50 PM
2	0.4571	0.1680mg/L	50uL	1.000		TC 0.1 - 20 ppm.2025_06_27_13_27_34.cal	6/27/2025 2:33:00 PM

Mean Area	0.4890
Mean Conc.	0.1797mg/L

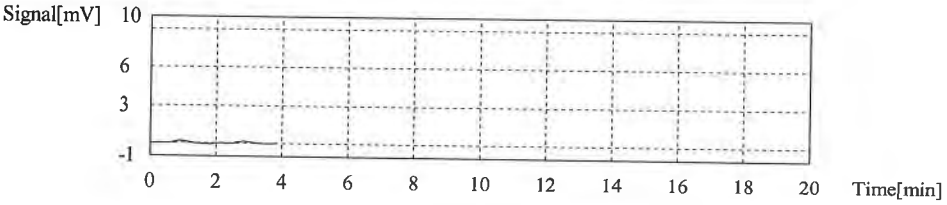

TOC-Control L Report

ALS
2025_06_27_001_PM.tlx

Instr.Information

Instrument Options: TOC/ASI/IC Unit/
Catalyst: Regular Sensitivity

Sample

Sample Name: Std. TC
Sample ID: 5 ppm
Origin: TC 0.1 - 20 ppm.cal
Status: Completed
Chk. Result:

Type	Anal.	Manual Dilution	Result
Unknown	TC	1.000	TC:5.244mg/L

1. Det

Anal.: TC

No.	Area	Conc.	Inj. Vol.	Aut. Dil.	Ex.	Cal. Curve	Date / Time
1	14.28	5.248mg/L	50uL	1.000		TC 0.1 - 20 ppm.2025_06_27_13_27_34.cal	6/27/2025 2:37:36 PM
2	14.26	5.241mg/L	50uL	1.000		TC 0.1 - 20 ppm.2025_06_27_13_27_34.cal	6/27/2025 2:40:04 PM

Mean Area: 14.27
Mean Conc.: 5.244mg/L

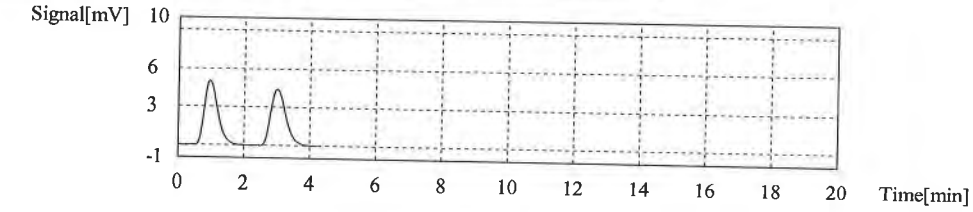

6/27/2025 3:04:38 PM

Automation Service Co.,Ltd.
Head Office : 929,929/1 Soi Pattanakarn 30, Pattanakarn Road, Suanluang, Bangkok
Tel: 02-319-9994
www.automation.co.th

Sales & Service Center
Rayong : 1/15 Huaypong Rd., Muang, Rayong 21150 [T. 038-692-152]
Lamphun : 122/5 M.4, Ban Klang, Muang, Lamphun 51000 [T. 053-581-876]
Prachinburi : 688 M.10, Thatum, Srimahaphote, Prachinburi 25140 [T. 037-208-880]

MTOC : L-0618/2025 Report No. : ALS-799

ASI Maintenance Report

Instrument	: Automatic Sample Injector	Measuring	: Vial 40 mL
Model	: ASI-L	Place of Installation	: -
Serial No.	: H57415200799	Department	: LABOLATORY
Manufacture	: Shimadzu		

Customer ALS Laboratory Group (Thailand) Co.,Ltd.
104 Phatthanakan 40, Phatthanakan Rd.,
Khwaen Suan Luang, Khet Suan Luang,
Bangkok 10250 Thailand

Date of Maintenance : 27 / 06 / 2025

REVIEW BY Ubon S.
APPROVED BY Sirilak B
NEXT CAL. DATE 27/6/26

Ambient Condition : Temperature 25.5 ± 5 °C
: Humidifier 58 ± 15 %RH

Maintenance By : Teeraphat Kamlungkua
(Mr. Teeraphat Kamlungkua)
Technician

Approved By :
(Mr. Nipon Phungsomsak)
Technician Manager

User Name : Sirilak B.
(Mr. Miss Sirilak Bunnak.)

SHIMADZU ANALYZER
1/3

Automation Service Co.,Ltd.

Head Office : 929,929/1 Soi Pattanakarn 30, Pattanakarn Road, Suanluang, Bangkok
Tel: 02-319-9994
www.automation.co.th

Sales & Service Center
Rayong : 1/15 Huaypong Rd., Muang, Rayong 21150 [T. 038-692-152]
Lamphun : 122/5 M.4, Ban Klang, Muang, Lamphun 51000 [T. 053-581-876]
Prachinburi : 688 M.10, Thatum, Srimahaphote, Prachinburi 25140 [T. 037-208-880]

MTOC : L-0618/2025

Report No. : ALS-799

Maintenance Sheet

Customer : ALS Laboratory Date : 27 / 06 / 2025

Model : ASI-L Serial No. H57415200799

Item	Carry out maintenance work	Result	Exchange	Comment
1.	Arm Drive section	O.K.		
	Check Arm Drive Belt for wear and tension	O.K.		
	Check grease of Screw Arm Drive	O.K.		
2.	Rinse pump (only ASI-V 24ml, 40ml)	O.K.		
	Check pump rate(>40mL/min)	O.K.		
	Check pump and tube connection for leakage	O.K.		
	Check if outlet flow is in proper condition	O.K.		
3.	Check and if necessary exchange consumable, Maintenance parts	O.K.		See appropriate list of maintenance parts
4.	Check Stirrer [When installed]	O.K.		
5.	Verify ASI function via mechanical check	O.K.		

Inspection by : Teeraphat Kamlungkua

(Mr. Teeraphat Kamlungkua)
Technician

Automation Service Co.,Ltd.
Head Office : 929,929/1 Soi Pattanakarn 30, Pattanakarn Road, Suanluang, Bangkok
Tel: 02-319-9994
www.automation.co.th

Sales & Service Center
Rayong : 1/15 Huaypong Rd., Muang, Rayong 21150 [T. 038-692-152]
Lamphun : 122/5 M.4, Ban Klang, Muang, Lamphun 51000 [T. 053-581-876]
Prachinburi : 688 M.10, Thatum, Srimahaphote, Prachinburi 25140 [T. 037-208-880]

MTOC : L-0618/2025 Report No. : ALS-799

List of Consumable, Maintenance parts

Pos.	Part Number	Part Name	Result	Exchange	Recommended Interval
1.	017-27021-01	Grease Paste, Lubricant 100g	O.K.	√	1 time per year
2.	032-22661-02	Belt, 60S2m596, Arm Drive	O.K.		1 time per year Depending on condition
3.	034-03067-02	Spring, F-642, Arm Drive	O.K.		Depending on condition
4.	042-00405-11	Pump Head, for ASI Rinse Pump (only ASI-V 24mL, 40mL)	O.K.		After 300 h of operating
5.	638-41448-01	Std. Needle Type1 24mL, 40mL* (for tube 2, 1x1, 6),[Sparge needle]	N/A		Depending on condition
6.	638-41448-02	Std. Needle Type1 125mL* (for tube 2, 1x1, 6)	N/A		Depending on condition
7.	631-41660-03	Flare Pipe 2x1,5x700mm* (for Standard Needle Type1 24mL,40mL, 125mL)	N/A		Depending on condition (may cut to origin length 600mm)
8.	638-41450-01	Needle for Suspended Particles,* 0,8mm (only ASI-V 24mL, 40mL)	N/A		Depending on condition
9.	638-41450-01	Std. Needle Type2 125mL* (for tube 1,4x0,9)	N/A		Depending on condition
10.	638-41472-01	Std. Needle Type2 24mL, 40mL* (for tube 1,4x0,9)	O.K.		Depending on condition
11.	631-41660-02	Flare Pipe 1,4x0,9x600mm* (for Suspended + Needle Type2)	O.K.		Depending on condition
12.	638-41449-01	Double Needle , only 24mL,40mL (simultaneous sparge type)*	N/A		Depending on condition
13.	631-41660-01	Flare Pipe 1,1x0,6x600mm* (for Double Needle 24mL,40mL)	N/A		Depending on condition

***Note: needed parts depending on installed needle types!**

Inspection by : Teeraphat Kamlungkua

(Mr. Teeraphat Kamlungkua)
Technician

© 2024 by Agilent Technologies

Certificate of System Qualification

GC-OQ + GCMS-OQ

System ID:	GM-10
Organization Name:	ALS Laboratory Group (Thailand) Co., Ltd.
Organization Location:	104 Patthanakarn 40, Patthanakarn Rd., Kwang Suan Luang, Khet Suan Luang, Bangkok 10250
Date:	November 21, 2024 2:12:44 PM
EQP Name:	AgilentRecommended , AgilentRecommended
EQP Revision:	GC.02.55, GCMS.02.56
Overall Qualification Status:	Pass

REVIEW BY Suchada T.

APPROVED BY Nart Sm

NEXT CAL. DATE 21-May-26

CDS Logon Verification - GC

Logon: asbkk.env03

Overall CDS Logon Verification Test Status

Pass

System Inspection and Basic Safety and Operation

Name: 7890

Setpoint Status: **Pass**

Overall System Inspection and Basic Safety and Operation Test Status

Pass

Inlet Pressure Accuracy

Name: 7890

Front MMI

Setpoint Status: **Pass**

	Setpoint		Actual	
Inlet Pressure:	25.0	psi	25.2	psi
Accuracy:			0.2	psi
Agilent Recommended:			<= 1.2	

© 2024 by Agilent Technologies

Overall Inlet Pressure Accuracy Test Status

Pass

GC Oven Temperature Accuracy

Name:	7890					
Setpoint Status:	**Pass**					
Zone:	Oven					
	Setpoint/Actual					
Temperature:	230.0	228.2	°C			
Accuracy:		-1.8	°C			
Agilent Recommended:	>=	-1.0	% setpoint in K	(	-5.0	°C)
	<=	1.0	% setpoint in K	(	5.0	°C)

Setpoint Status:	**Pass**					
Zone:	Oven					
	Setpoint/Actual					
Temperature:	100.0	100.7	°C			
Accuracy:		0.7	°C			
Agilent Recommended:	>=	-1.0	% setpoint in K	(	-3.7	°C)
	<=	1.0	% setpoint in K	(	3.7	°C)

Overall GC Oven Temperature Accuracy Test Status

Pass

NOTE: This test's 2 comment(s) and 0 deviation(s) are available in the Attachments section.

GC Oven Temperature Stability

Name:	7890		
Setpoint Status:	**Pass**		
	Setpoint/Average		
Temperature:	100.0	100.7333	°C
Stability:		0.1	°C
Agilent Recommended:	<=	0.5	

© 2024 by Agilent Technologies

Overall GC Oven Temperature Stability Test Status

Pass

NOTE: This test's 1 comment(s) and 0 deviation(s) are available in the Attachments section.

Tune EI

Tested Combination1	Front	MMI	/	External	TQ
Name:	7000D				
Setpoint Status:	**Pass**				
Filament:	1				
Setpoint Status:	**Pass**				
Filament:	2				

Overall Tune EI Test Status

Pass

Scouting Run

Tested Combination1	Front	MMI	/	External	TQ
	Injection Tower				
Name:	7693A				
Source:	EI - Extractor				
Setpoint Status:	**Completed**				
Injection Volume on Column:	1.0 uL				

Overall Scouting Run Status

Completed

Instrument Detection Limit

Tested Combination1	Front	MMI	/	External	TQ
	Injection Tower				
Name:	7693A				
Source:	EI - Extractor				

Setpoint Status:	**Pass**	
Injection Volume on Column:	1.0 uL	
	Area	Retention Time
Minimum RSD:	4.58 %	0.01 %
Agilent Recommended:	<= 12.00	<= 1.00
Status:	Pass	Pass
Instrument Detection Limit:	1.54238 fg	
Agilent Recommended:	<= 4.03800	
Status:	Pass	

Overall Instrument Detection Limit Test Status

Pass

Mass Ratio Precision

Tested Combination1	Front Injection Tower	MMI	/ External	TQ
Name:	7693A			
Source:	EI - Extractor			

Setpoint Status:	**Pass**	
Injection Volume on Column:	0.5 uL	
	Area Mass 1 Abundance*s	Mass Ratio
RSD:	2.23 %	0.10 %
Agilent Recommended:	<= 5.00	<= 5.00
	Pass	Pass

Overall Mass Ratio Precision Test Status

Pass

Instrument Details

Purpose

This section describes the as found system configuration.

Details

System

System ID	GM-10
Manufacturer	Agilent Technologies
Name	7890
Flow Data Input	Manual Data
Temperature Data Input	Manual Data or Other Data Logging

Tested Combination1

Injection Technique	Injection Tower
Inlet	Front
Detector	External
LTM Included?	No

Sampler 1

Manufacturer	Agilent Technologies
Type	Injection Tower
Name	7693A
Model Number	G4513A
Serial Number	CN18180003
Firmware Revision	A.11.02
Usage	Sample Injection
Location	Front
Syringe Volume (µL)	10

Sampler 2

Manufacturer	Agilent Technologies
Type	Tray
Name	7693A
Model Number	G4514A
Serial Number	CN18170137
Firmware Revision	A.11.03
Vial Heater	Not installed

Mainframe 1

Manufacturer	Agilent Technologies
Name	7890
Model Number	G3442B
Serial Number	CN18153080
Firmware Revision	B.02.05
Oven Type	Standard

Inlet 1

Manufacturer	Agilent Technologies
Name	7890
Type	MMI
Location	Front
Carrier Gas	Helium
Control Type	Electronic Pressure Control (EPC)
Purged Inlet	Yes

Inlet 2

Manufacturer	Agilent Technologies
Name	7890
Type	SSL
Location	Back
Carrier Gas	Helium
Control Type	Electronic Pressure Control (EPC)
Purged Inlet	Yes

Detector 1

Manufacturer	Agilent Technologies
Name	Mass Spectrometer
Type	Mass Spectrometer
Location	External

Mass Spectrometer 1

Manufacturer	Agilent Technologies
Type	TQ
Name	7000D
Model Number	G7000D
Serial Number	US1826U108
Firmware Revision	G.7000.085A
High Vacuum System	Turbo Pump
Liquid Injection Scouting Run Standard	OFN Std

MS EI Source 1

Manufacturer	Agilent Technologies
Source Type	EI - Extractor
Number of filaments	2

© 2024 by Agilent Technologies

Electronic Signature

Purpose

This signature page was created and published because the ACE sign-off action was executed, which is valid for the entire document, including attachments. The ACE sign-off is an electronic signature that requires two distinct identification components: unique username and personal password. The Agilent representative who has delivered this service understands the meaning and legal status of an electronic signature. As a trained official operator, the Agilent representative has a unique password and logon to access ACE and electronically sign this document. (Other e-signatures can be applied to this document using a Document Content Management or other suitable method defined in your data access and control procedures.)

Details

Full Name of Signer:	Supasak Nimsongtham
Logged On User Name:	supasak.nimsongtham@agilent.com
Signature Creation Date:	November 21, 2024
Reason for Signature:	Executed protocol and published this original version of document

ACE Self Qualification Status

The installed version of ACE used to deliver this service passed qualification; the results conform with expected values. The self qualification summary report is available in the session folder location SDS\ClearStore\AceSelfQualification.

Regulatory Disclaimer

This document provides a protocol to verify and record instrument configuration and evidence of proper operation. It has been prepared from our interpretation of applicable regulations as well as industry best practices. The document is designed to provide an important component of a complete compliance package. Validation depends upon many factors and use of this protocol alone does not assure compliance. Agilent Technologies makes no promises or representations as to its sufficiency for any specific regulatory program.

Warranty

Agilent Technologies makes no warranty of any kind to this material, including but not limited to, the implied warranties or merchantability and fitness for a particular purpose. Agilent Technologies shall not be liable for errors contained herein or for incidental or consequential damages in connection with the furnishing, performance, or use of this material.

© 2024 by Agilent Technologies

User Name: supasak.nimsongtham
Report Generated by Hostname: 5CG1115HKC

System Id: GM-10
Print Date: November 21, 2024 2:12:46 PM

GM-10 2024 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
November 21, 2024 11:58:17 AM	Audit	SessionCreated	Session	Host Name: 5CG1115HKC, Drive Serial Number: C2031778
November 21, 2024 11:58:17 AM	start	Configuration	Session	None
November 21, 2024 11:58:17 AM	Audit	Entitlement	Licensing	User is FieldEngineer and does not require an unlock code
November 21, 2024 12:01:59 PM	Audit	EqpLoaded	Session	EQP details for primary technique [Gc] - File path: [ProtocolPacks/Gc/Configurations/02.55/Gc.02.55.eqp], EQP File Name: [Gc.02.55.eqp], EQP Name: [AgilentRecommended],Protocol Revision :[Gc.02.55] EQP details for hyphenated technique [GcMs] - File path: [ProtocolPacks/GcMs/Configurations/02.56/GcMs.02.56.eqp], EQP File Name: [GcMs.02.56.eqp], EQP Name: [AgilentRecommended]
November 21, 2024 12:02:04 PM	End	Configuration	Session	None
November 21, 2024 12:02:12 PM	start	Qualification	Session	OQ
November 21, 2024 12:02:12 PM	start	Execution	CDS Logon Verification - GC - 7890: - Qualitative test	None
November 21, 2024 12:03:09 PM	End	Execution	CDS Logon Verification - GC - 7890: - Qualitative test	Run Count : 1

© 2024 by Agilent Technologies

User Name: supasak.nimsongtham
Report Generated by Hostname: 5CG1115HKC

System Id: GM-10
Print Date: November 21, 2024 2:12:46 PM

GM-10 2024 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
November 21, 2024 12:03:11 PM	start	Execution	System Inspection and Basic Safety and Operation - 7890: - Qualitative Test - No setpoints associated	None
November 21, 2024 12:03:20 PM	End	Execution	System Inspection and Basic Safety and Operation - 7890: - Qualitative Test - No setpoints associated	Run Count : 1
November 21, 2024 12:03:23 PM	start	Execution	Inlet Pressure Accuracy - Front MMI: - Pressure Controlled Inlet - S: 25.0 psi - L: <= 1.2 psi	None
November 21, 2024 12:03:28 PM	End	Execution	Inlet Pressure Accuracy - Front MMI: - Pressure Controlled Inlet - S: 25.0 psi - L: <= 1.2 psi	Run Count : 1
November 21, 2024 12:03:30 PM	start	Execution	GC Oven Temperature Accuracy - 7890: - Temperature : Oven - S: 230.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	None
November 21, 2024 12:06:02 PM	Audit	Data	GC Oven Temperature Accuracy - 7890: - Temperature : Oven - S: 230.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	Manual Data Entry
November 21, 2024 12:06:05 PM	End	Execution	GC Oven Temperature Accuracy - 7890: - Temperature : Oven - S: 230.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	Run Count : 1
November 21, 2024 12:06:07 PM	start	Execution	GC Oven Temperature Accuracy - 7890: - Temperature : Oven - S: 100.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	None
November 21, 2024 12:06:20 PM	Audit	Data	GC Oven Temperature Accuracy - 7890: - Temperature : Oven - S: 100.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	Manual Data Entry

© 2024 by Agilent Technologies

User Name: supasak.nimsongtham
Report Generated by Hostname: 5CG1115HKC

System Id: GM-10
Print Date: November 21, 2024 2:12:46 PM

GM-10 2024 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
November 21, 2024 12:06:23 PM	End	Execution	GC Oven Temperature Accuracy - 7890: - Temperature : Oven - S: 100.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	Run Count : 1
November 21, 2024 12:06:25 PM	start	Execution	GC Oven Temperature Stability - 7890: - Temperature : Oven - S: 100.0°C - L: <= 0.5°C	None
November 21, 2024 12:07:10 PM	Audit	Data	GC Oven Temperature Stability - 7890: - Temperature : Oven - S: 100.0°C - L: <= 0.5°C	Manual Data Entry
November 21, 2024 12:07:14 PM	End	Execution	GC Oven Temperature Stability - 7890: - Temperature : Oven - S: 100.0°C - L: <= 0.5°C	Run Count : 1
November 21, 2024 12:07:16 PM	start	Execution	Tune EI - 7000D TQ: - Source: - EI - Extractor Filament 1 (Qualitative - No setpoints associated)	None
November 21, 2024 12:07:26 PM	End	Execution	Tune EI - 7000D TQ: - Source: - EI - Extractor Filament 1 (Qualitative - No setpoints associated)	Run Count : 1
November 21, 2024 12:07:28 PM	start	Execution	Tune EI - 7000D TQ: - Source: - EI - Extractor Filament 2 (Qualitative - No setpoints associated)	None
November 21, 2024 12:07:39 PM	End	Execution	Tune EI - 7000D TQ: - Source: - EI - Extractor Filament 2 (Qualitative - No setpoints associated)	Run Count : 1
November 21, 2024 12:07:41 PM	start	Execution	Scouting Run - Injection Tower, Front MMI, TQ: - Source: - EI - Extractor- Part of GCMS System Preparation	None

Date: November 21, 2024 2:12:44 PM
System ID: GM-10

User Name: supasak.nimsongtham
Report Generated by Hostname: 5CG1115HKC

System Id: GM-10
Print Date: November 21, 2024 2:12:46 PM

GM-10 2024 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
November 21, 2024 12:08:53 PM	Audit	Data	Scouting Run - Injection Tower, Front MMI, TQ: - Source: - EI - Extractor- Part of GCMS System Preparation	Data files Path : C:\GM-10 OQ2024\SC001.D
November 21, 2024 12:09:23 PM	Audit	Reporting	Reintegration	Reintegration Count: 1 -- [Integration Type: Injection;Baseline Correction Mode: Advanced;Initial Slope Sensitivity: 10;Initial Peak Width: 0.01;Initial Area Reject: 0;Initial Height Reject: 50;Integration: Off at 0;Integration: On at 4]
November 21, 2024 12:09:50 PM	End	Execution	Scouting Run - Injection Tower, Front MMI, TQ: - Source: - EI - Extractor- Part of GCMS System Preparation	Run Count : 1
November 21, 2024 12:09:53 PM	start	Execution	Instrument Detection Limit - Injection Tower, Front MMI, TQ: - Source: - EI - Extractor - RSD L (Area): <= 12.00% - RSD L (Ret. Time): <= 1.00%	None
November 21, 2024 12:16:46 PM	Audit	Data	Instrument Detection Limit - Injection Tower, Front MMI, TQ: - Source: - EI - Extractor - RSD L (Area): <= 12.00% - RSD L (Ret. Time): <= 1.00%	Data files Path : C:\GM-10 OQ2024\IDL001.D
November 21, 2024 12:16:46 PM	Audit	Data	Instrument Detection Limit - Injection Tower, Front MMI, TQ: - Source: - EI - Extractor - RSD L (Area): <= 12.00% - RSD L (Ret. Time): <= 1.00%	Data files Path : C:\GM-10 OQ2024\IDL002.D

© 2024 by Agilent Technologies

User Name: supasak.nimsongtham
Report Generated by Hostname: 5CG1115HKC

System Id: GM-10
Print Date: November 21, 2024 2:12:46 PM

GM-10 2024 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
November 21, 2024 12:16:46 PM	Audit	Data	Instrument Detection Limit - Injection Tower, Front MMI, TQ: - Source: - EI - Extractor - RSD L (Area): <= 12.00% - RSD L (Ret. Time): <= 1.00%	Data files Path : C:\GM-10 OQ2024\IDL003.D
November 21, 2024 12:16:46 PM	Audit	Data	Instrument Detection Limit - Injection Tower, Front MMI, TQ: - Source: - EI - Extractor - RSD L (Area): <= 12.00% - RSD L (Ret. Time): <= 1.00%	Data files Path : C:\GM-10 OQ2024\IDL004.D
November 21, 2024 12:16:47 PM	Audit	Data	Instrument Detection Limit - Injection Tower, Front MMI, TQ: - Source: - EI - Extractor - RSD L (Area): <= 12.00% - RSD L (Ret. Time): <= 1.00%	Data files Path : C:\GM-10 OQ2024\IDL005.D
November 21, 2024 12:16:47 PM	Audit	Data	Instrument Detection Limit - Injection Tower, Front MMI, TQ: - Source: - EI - Extractor - RSD L (Area): <= 12.00% - RSD L (Ret. Time): <= 1.00%	Data files Path : C:\GM-10 OQ2024\IDL006.D
November 21, 2024 12:16:47 PM	Audit	Data	Instrument Detection Limit - Injection Tower, Front MMI, TQ: - Source: - EI - Extractor - RSD L (Area): <= 12.00% - RSD L (Ret. Time): <= 1.00%	Data files Path : C:\GM-10 OQ2024\IDL007.D
November 21, 2024 12:16:47 PM	Audit	Data	Instrument Detection Limit - Injection Tower, Front MMI, TQ: - Source: - EI - Extractor - RSD L (Area): <= 12.00% - RSD L (Ret. Time): <= 1.00%	Data files Path : C:\GM-10 OQ2024\IDL008.D
November 21, 2024 12:16:47 PM	Audit	Data	Instrument Detection Limit - Injection Tower, Front MMI, TQ: - Source: - EI - Extractor - RSD L (Area): <= 12.00% - RSD L (Ret. Time): <= 1.00%	Data files Path : C:\GM-10 OQ2024\IDL009.D

User Name: supasak.nimsongtham
Report Generated by Hostname: 5CG1115HKC

System Id: GM-10
Print Date: November 21, 2024 2:12:46 PM

GM-10 2024 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
November 21, 2024 12:16:47 PM	Audit	Data	Instrument Detection Limit - Injection Tower, Front MMI, TQ: - Source: - EI - Extractor - RSD L (Area): <= 12.00% - RSD L (Ret. Time): <= 1.00%	Data files Path : C:\GM-10 OQ2024\IDL010.D
November 21, 2024 12:18:15 PM	Audit	Reporting	Reintegration	Reintegration Count: 1 -- [Integration Type: Injection;Baseline Correction Mode: Advanced;Initial Slope Sensitivity: 10;Initial Peak Width: 0.01;Initial Area Reject: 0;Initial Height Reject: 50;Integration: Off at 0;Integration: On at 4]
November 21, 2024 12:22:43 PM	End	Execution	Instrument Detection Limit - Injection Tower, Front MMI, TQ: - Source: - EI - Extractor - RSD L (Area): <= 12.00% - RSD L (Ret. Time): <= 1.00%	Run Count : 1
November 21, 2024 12:22:52 PM	start	Execution	Mass Ratio Precision - Injection Tower, Front MMI, TQ: - Source: EI - Extractor - L (RSD): <= 5.00%	None
November 21, 2024 12:27:38 PM	Audit	Data	Mass Ratio Precision - Injection Tower, Front MMI, TQ: - Source: EI - Extractor - L (RSD): <= 5.00%	Data files Path : C:\GM-10 OQ2024\MRP002.D
November 21, 2024 12:27:38 PM	Audit	Data	Mass Ratio Precision - Injection Tower, Front MMI, TQ: - Source: EI - Extractor - L (RSD): <= 5.00%	Data files Path : C:\GM-10 OQ2024\MRP003.D
November 21, 2024 12:27:38 PM	Audit	Data	Mass Ratio Precision - Injection Tower, Front MMI, TQ: - Source: EI - Extractor - L (RSD): <= 5.00%	Data files Path : C:\GM-10 OQ2024\MRP004.D

Page 6 / 7

© 2024 by Agilent Technologies

User Name: supasak.nimsongtham
Report Generated by Hostname: 5CG1115HKC

System Id: GM-10
Print Date: November 21, 2024 2:12:46 PM

GM-10 2024 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
November 21, 2024 12:27:38 PM	Audit	Data	Mass Ratio Precision - Injection Tower, Front MMI, TQ: - Source: EI - Extractor - L (RSD): <= 5.00%	Data files Path : C:\GM-10 OQ2024\MRP005.D
November 21, 2024 12:27:39 PM	Audit	Data	Mass Ratio Precision - Injection Tower, Front MMI, TQ: - Source: EI - Extractor - L (RSD): <= 5.00%	Data files Path : C:\GM-10 OQ2024\MRP006.D
November 21, 2024 12:27:39 PM	Audit	Data	Mass Ratio Precision - Injection Tower, Front MMI, TQ: - Source: EI - Extractor - L (RSD): <= 5.00%	Data files Path : C:\GM-10 OQ2024\MRP007.D
November 21, 2024 12:33:20 PM	Audit	Reporting	Reintegration	Reintegration Count: 1 -- [Integration Type: Injection;Baseline Correction Mode: Advanced;Initial Slope Sensitivity: 10;Initial Peak Width: 0.01;Initial Area Reject: 0;Initial Height Reject: 50000;Integration: Off at 0;Integration: On at 4]
November 21, 2024 12:36:42 PM	End	Execution	Mass Ratio Precision - Injection Tower, Front MMI, TQ: - Source: EI - Extractor - L (RSD): <= 5.00%	Run Count : 1
November 21, 2024 12:37:11 PM	End	Qualification	Session	OQ
November 21, 2024 12:37:11 PM	start	Reporting	Session	None
November 21, 2024 1:11:02 PM	Audit	Reporting	Session	Report Generated : Certificate
November 21, 2024 1:37:20 PM	Audit	Reporting	Session	Report Generated : Report