



๑๘ มกราคม ๒๕๖๗

เรื่อง ต่ออายุหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน

เรียน กรรมการผู้จัดการ บริษัท สเปเชียล แล็บ เอ็นไว แอนด์ คอนซัลแตนท์ จำกัด

อ้างถึง คำขอขึ้นทะเบียน/ต่ออายุ/เปลี่ยนแปลงบุคลากร และชนิดสารมลพิษของห้องปฏิบัติการวิเคราะห์เอกชน
ลงวันที่ ๑ พฤศจิกายน ๒๕๖๖

สิ่งที่ส่งมาด้วย เอกสารแนบท้ายหนังสือต่ออายุรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน
บริษัท สเปเชียล แล็บ เอ็นไว แอนด์ คอนซัลแตนท์ จำกัด จำนวน ๒ แผ่น

ตามหนังสือที่อ้างถึง บริษัท สเปเชียล แล็บ เอ็นไว แอนด์ คอนซัลแตนท์ จำกัด ห้องปฏิบัติการ
วิเคราะห์เอกชน เลขทะเบียน ว-๑๓๓ สถานที่ตั้งเลขที่ ๔๗/๙๑-๙๓ หมู่ที่ ๓ ตำบลท่าอิฐ อำเภอปากเกร็ด
จังหวัดนนทบุรี ต่อกรมโรงงานอุตสาหกรรม นั้น

กรมโรงงานอุตสาหกรรมพิจารณาแล้ว ให้บริษัท สเปเชียล แล็บ เอ็นไว แอนด์ คอนซัลแตนท์ จำกัด
ต่ออายุหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน โดยมีองค์ประกอบดังนี้

ก. ผู้ควบคุมดูแลห้องปฏิบัติการวิเคราะห์

- | | |
|--------------------------|----------------------------|
| ๑) นางสาวฟาติฮะห์ สุลหลง | ทะเบียนเลขที่ ว-๑๓๓-ค-๐๐๐๑ |
| ๒) นางสาวอัศวานี ยูโซะ | ทะเบียนเลขที่ ว-๑๓๓-ค-๐๐๐๒ |
| ๓) นายมะปารี อาแวกือจิ | ทะเบียนเลขที่ ว-๑๓๓-ค-๐๐๐๓ |

ข. เจ้าหน้าที่ประจำห้องปฏิบัติการวิเคราะห์

- | | |
|------------------------------|----------------------------|
| ๑) นางสาวบุศรียะ ยีชา | ทะเบียนเลขที่ ว-๑๓๓-จ-๐๐๐๒ |
| ๒) นางสาวนุรีไลลา มะแซ | ทะเบียนเลขที่ ว-๑๓๓-จ-๐๐๐๓ |
| ๓) นางสาวชาอีรา สาแม | ทะเบียนเลขที่ ว-๑๓๓-จ-๐๐๐๔ |
| ๔) นางสาวนุรีสา สอเลาะห์ | ทะเบียนเลขที่ ว-๑๓๓-จ-๐๐๐๕ |
| ๕) นางสาวณัฐกานต์ บากาโชติ | ทะเบียนเลขที่ ว-๑๓๓-จ-๐๐๐๖ |
| ๖) นางสาวซารีนานา บัวซ์ | ทะเบียนเลขที่ ว-๑๓๓-จ-๐๐๐๗ |
| ๗) นางสาวบรั๊กกีส์ หะยีกือจิ | ทะเบียนเลขที่ ว-๑๓๓-จ-๐๐๐๘ |
| ๘) นางสาวโนร์โซเฟีย มะนอ | ทะเบียนเลขที่ ว-๑๓๓-จ-๐๐๐๙ |
| ๙) นางสาวอามีรา แวหะแน | ทะเบียนเลขที่ ว-๑๓๓-จ-๐๐๑๐ |
| ๑๐) นางสาวนุรฮัยมี อาแวกือจิ | ทะเบียนเลขที่ ว-๑๓๓-จ-๐๐๑๑ |
| ๑๑) นางสาวอิฟตีซาน หะมะ | ทะเบียนเลขที่ ว-๑๓๓-จ-๐๐๑๒ |
| ๑๒) นายเสรี จันทวี | ทะเบียนเลขที่ ว-๑๓๓-จ-๐๐๑๓ |

ค. ขอบข่ายสารมลพิษที่ได้รับขึ้นทะเบียนให้วิเคราะห์ในน้ำเสีย ตามสิ่งที่ส่งมาด้วย

หนังสือฉบับนี้จะหมดอายุในวันที่ ๒๕ มกราคม ๒๕๗๐ หากประสงค์จะต่ออายุหนังสือ
รับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน ให้ยื่นคำขอต่ออายุพร้อมเอกสารประกอบคำขอต่อกรมโรงงาน
อุตสาหกรรมภายใน ๓๐ วัน ก่อนวันสิ้นอายุของหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน ทั้งนี้
สามารถยื่นคำขอผ่านระบบอิเล็กทรอนิกส์ได้ที่หน้าเว็บไซต์กรมโรงงานอุตสาหกรรม

จึงเรียนมาเพื่อทราบ

ขอแสดงความนับถือ



(นายศิระ จันทรเจ็ด)

นักวิทยาศาสตร์เชี่ยวชาญ วิชาการการแทน
ผู้อำนวยการกองวิจัยและเตือนภัยมลพิษโรงงาน
ปฏิบัติราชการแทนอธิบดีกรมโรงงานอุตสาหกรรม

กองวิจัยและเตือนภัยมลพิษโรงงาน

กลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษและทะเบียนห้องปฏิบัติการ

โทร. ๐ ๒๔๓๐ ๖๓๑๒ ต่อ ๒๑๐๓-๕

โทรสาร ๐ ๒๔๓๐ ๖๓๑๒ ต่อ ๒๑๙๙

ไปรษณีย์อิเล็กทรอนิกส์ saraban@diw.mail.go.th



เอกสารแนบท้ายหนังสือต่ออายุรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน

บริษัท สเปเชียล แล็บ เอ็นไว แอนด์ คอนซัลแตนท์ จำกัด

เลขทะเบียน ว-๑๓๓

ที่ อก ๐๓๑๐(๑)/ ๕๐๖

ลงวันที่ ๑๘ มกราคม ๒๕๖๗

ขอขยายสารมลพิษที่ได้รับขึ้นทะเบียนจากกรมโรงงานอุตสาหกรรม จำนวน ๒๖ รายการ

น้ำเสีย จำนวน 26 รายการ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
1	Arsenic	Digestion, Hydride Generation/Atomic Absorption Spectrometric Method ^[2]
2	Barium	Digestion, Direct Nitrous Oxide-Acetylene Flame Method ^[2]
3	Biochemical Oxygen Demand	1) 5-Day BOD Test, Azide Modification Method ^[2] 2) 5-Day BOD Test, Membrane Electrode Method ^[2]
4	Cadmium	Digestion, Direct Air-Acetylene Flame Method ^[2]
5	Chemical Oxygen Demand	Closed Reflux, Colorimetric Method ^[2]
6	Color	ADMI Weighted-Ordinate Spectrophotometric Method ^[2]
7	Copper	Digestion, Direct Air-Acetylene Flame Method ^[2]
8	Cyanide	Distillation, Colorimetric Method ^[2]
9	Formaldehyde	Distillation, Colorimetric Method ^[1]
10	Free Chlorine	DPD Colorimetric Method ^[2]
11	Hexavalent Chromium	Colorimetric Method ^[2]
12	Lead	Digestion, Direct Air-Acetylene Flame Method ^[2]
13	Manganese	Digestion, Direct Air-Acetylene Flame Method ^[2]
14	Mercury	Digestion, Cold-Vapor Atomic Absorption Spectrometric Method ^[2]
15	Nickel	Digestion, Direct Air-Acetylene Flame Method ^[2]
16	Oil & Grease	Liquid-Liquid, Partition-Gravimetric Method ^[2]
17	pH	Electrometric Method ^[2]
18	Phenols	1) Distillation, Chloroform Extraction Method ^[2] 2) Distillation, Direct Photometric Method ^[2]
19	Selenium	Digestion, Hydride Generation/Atomic Absorption Spectrometric Method ^[2]
20	Sulfide	Iodometric Method ^[2]
21	Temperature	Laboratory and Field Methods ^[2]
22	Total Dissolved Solids	Dried at 180 °C ^[2]

3mg/l

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
23	Total Kjeldahl Nitrogen	Macro-Kjeldahl Method ^[2]
24	Total Suspended Solids	Dried from 103-105 °C ^[2]
25	Trivalent Chromium	Digestion, Direct Air-Acetylene Flame Method; Colorimetric Method; Calculation ^[2]
26	Zinc	Digestion, Direct Air-Acetylene Flame Method ^[2] สมุ

เอกสารอ้างอิง

1. สมาคมวิศวกรรมสิ่งแวดล้อมแห่งประเทศไทย. คู่มือวิเคราะห์น้ำเสีย. พิมพ์ครั้งที่ 4. กรุงเทพฯ: เรือนแก้วการพิมพ์, 2547.
2. APHA, AWWA, WEF. Standard Methods for the Examination of Water and Wastewater. 24th ed. Washington, DC: APHA, 2023.



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)

CORPORATE SERVICES 3 : EQUIPMENT CALIBRATION AND TESTING SERVICES

534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250

TEL. 0-2717-3000 FAX. 0-2719-9484

Certificate of Testing

Cert.No.: 26TW31

Page.: 1 of 2

Equipment :	DO Meter
Manufacturer :	Hanna
Model :	HI98193
Serial No. :	09120032101
ID No. :	LB-Eq-014
Received Date :	02 February 2026
Test Date :	03 February 2026
Reference :	2602-0045WN-1
Submitted by :	Special Lab Envi And Consultant Co.,Ltd 47/91-93 Moo 3 Thambon Tha-it, Pakkret, Nonthaburi 11120
Laboratory Condition :	Temperature (25 ± 5) °C Humidity (50 ± 20) %
Test Procedure :	In - house method : CP-CH9 by Comparison Technique with Azide Modification Method
Tested by :	Walalak Sirithean
Approved by :	<hr/> Approved Signatory
() Chakrit Waewwanjua () Ponpan Paipim (✓) Saithip Meangmai	
Issue Date :	03 February 2026



Cert.No.: 26TW31

Page.: 2 of 2

Condition of this result of calibration

1. Reference Standard Instruments :

This measurement result is traceable to the International System of Unit through the reference standards laboratory of Industrial Calibration Center, Technology Promotion Association (Thailand-Japan).

<u>Instruments</u>	<u>ID No.</u>	<u>Certificate No.</u>	<u>Due Date</u>
1. Burette	130BU10	25CG1126	18 Mar 2027
2. Balance	110RC001	25MM316	02 July 2026

2. Standard Material :-

<u>Material</u>	<u>Manufacturer</u>	<u>Lot.No.</u>	<u>Assay</u>
Sodium Thiosulfate 5-Hydrate AR	KEMAUS	2203162447	99.6%

Result : **Dissolved Oxygen Meter Adjustment With Air 100 %**

Dissolved Oxygen Probe No.: KC1N8943T

Titration Method (Azide Modification Method) (mg/L)	DO Meter Reading (mg/L)	Standard Deviation (mg/L)
8.20	8.20	0.0045

This report was certified only for the instrument we tested. It is allowable to use for study
Intend to use for advertising and referral purpose is prohibited. This report may not be reproduced
other in full, without written approval of the laboratory

-o0o-



CALIBRATION CERTIFICATE

Date of Issue Jun 17, 2025

Cert No. 25/2478

Order No. 25060343

Customer SPECIAL LAB ENVI AND CONSULTANT CO., LTD.
47/91 Moo 3, Tha-It, Pakkert, Nonthaburi 11120

Place of Calibration Laboratory Room

Description Oven

Model UF30

Serial No. B123.0544

ID.No. LB-Eq-047

Date of Receipt Jun 16, 2025

Date of Calibration Jun 16, 2025

Environment

Temperature (Min) 29.4 °C (Max) 30.8 °C

Relative Humidity (Min) 48.7 %rh (Max) 52.6 %rh

Calibration Method

WI-17 : The reference thermometer was placed into the chamber and measurement was performed based on AS-2853.

The temperature scale in use at this laboratory is the International Temperature Scale of 1990.

Standard Equipment	Serial No.	Certificate No.	Due Date
1) Data Acquisition Switch Unit with Sensor	MY49007789	QR25-0353	30 Jan 2026

This certificate is traceable to SI unit.


CALIBRATION CERTIFICATE

Date of Issue Jun 17, 2025

Cert No. 25/2478

Order No. 25060343

Results (without adjustment)

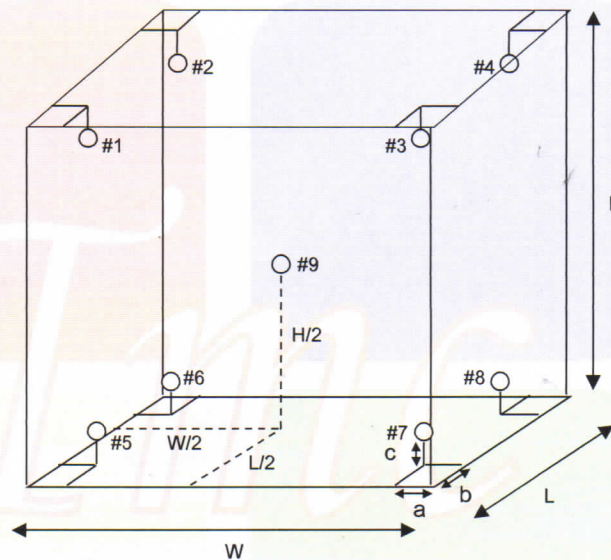

Position of reference thermometers were placed

Note.

- 1). Dimension (W x L x H) is 40 x 25 x 32 cm.
- 2). Stability - greatest one half of difference between max peak and min peak of each reference probe measured temperature obtained during the calibration interval.
- 3). Uniformity - the maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady state conditions. The reference sensor should preferably be located at the geometric center of the chamber.



CALIBRATION CERTIFICATE

Date of Issue Jun 17, 2025

Cert No. 25/2478

Order No. 25060343

Results (without adjustment)

Cal Point (°C)	UUC Setting (°C)	UUC Reading (°C)	Reference Thermometer (°C)		Stability \pm (°C)	Uniformity (°C)	Uncertainty \pm (°C)
104.0	104.0	104.0	Position 1	104.381	0.062	0.911	0.36
			Position 2	103.624			
			Position 3	103.718			
			Position 4	103.628			
			Position 5	103.579			
			Position 6	103.557			
			Position 7	103.569			
			Position 8	103.587			
			Position 9	103.513			

Cal Point (°C)	UUC Setting (°C)	UUC Reading (°C)	Reference Thermometer (°C)		Stability \pm (°C)	Uniformity (°C)	Uncertainty \pm (°C)
150.0	150.0	150.0	Position 1	150.997	0.115	1.597	0.50
			Position 2	149.610			
			Position 3	149.802			
			Position 4	149.659			
			Position 5	149.570			
			Position 6	149.512			
			Position 7	149.500			
			Position 8	149.743			
			Position 9	149.471			



CALIBRATION CERTIFICATE

Date of Issue Jun 17, 2025

Cert No. 25/2478

Order No. 25060343

Results (without adjustment)

Cal Point (°C)	UUC Setting (°C)	UUC Reading (°C)	Reference Thermometer (°C)		Stability ±(°C)	Uniformity (°C)	Uncertainty ±(°C)
180.0	180.0	180.0	Position 1	181.288	0.079	1.994	0.57
			Position 2	179.511			
			Position 3	179.762			
			Position 4	179.572			
			Position 5	179.506			
			Position 6	179.420			
			Position 7	179.327			
			Position 8	179.840			
			Position 9	179.353			

The stability and uniformity were taken into account in the measurement uncertainty stated.

The above results are valid exclusively for calibration samples as mentioned in this report.

This reported expanded uncertainty was based on a standard uncertainty multiplied by a coverage factor $k=2$, providing a level of confidence of approximately 95%. The uncertainty evaluation has been carried out in accordance with ONAC requirements.

APPROVED SIGNATORY :

D.M.

☐ MR. PRAJUCKPETCH THONGSOOKCHOTE

☒ MR. DAMRONG MULSING

☐ MR. JATURAPAT THONGSOOKCHOTE



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL.0-2717-3000-29 FAX.0-2719-9484



Certificate of Calibration

Cert.No.: 25CH644

Page.: 1 of 3

Equipment : pH Meter
Manufacturer : Horiba
Model : LAQUAact-PH130
Serial No. : D08C0004
ID No. : -
Condition As-Received: Used Item
Received Date : 02 June 2025
Calibration Date : 05 June 2025
Reference : 2506-0035WN-1
Submitted by : Special Lab Envi And Consultant Co.,Ltd
47/91-93 Moo 3 Thambon Tha-it, Pakkret
Nonthaburi 11120

Ambient Temperature : (25 ± 2.5) °C
Relative Humidity : (50 ± 15) %
Calibration Procedure : In - house method :
- CP-CH5 by direct measurement with DC voltage standard and direct measurement with certified reference material (CRM)
- CP-CH8 by comparison with temperature standard

Calibrated by : Khit Ruttanaprapachai

Approved by : _____
Approved Signatory

() Chakrit Waewwanjua
() Ponpan Paipim
(✓) Saithip Meangmai

Issue Date : 6 June 2025

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.



Cert.No.: 25CH644

Page.: 2 of 3

Condition of this calibration result

1. Reference Standard Instrument

<u>Instrument</u>	<u>Serial No.</u>	<u>ID No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
1) Document Process Calibrator	43160066	130RC092	25E1217	17 Apr 2026
2) Ref. Standard Thermometer	2188080	130RC044	24I1022	16 Sep 2025

- This measurement result is traceable to SI through Technology Promotion Association (Thailand - Japan)

2. Certified Reference Materials : The measurement results are traceable to SI through CPA chem Ltd.,
ANSI-ASQ National Accreditation Board, Accredited No. AR-1835

<u>Buffer Solution</u>	<u>Manufacturer</u>	<u>Lot No.</u>	<u>Exp. date</u>
pH 4.007	CPA chem	1066665	18 Jan 2027
pH 6.865	CPA chem	940103	02 Nov 2025
pH 9.180	CPA chem	1066668	18 Jan 2026

3. This certificate is valid only to the item calibrated on date and place of calibration.

Calibration Results

Function : mV Measurement

Performing standard curve by Document Process Calibrator at pH (4,7,9)

Unit Under Calibration	Nominal Value	Standard Voltage Input	Actual Reading		Uncertainty of Measurement (±mV)	Coverage factor <i>k</i>
	pH	mV	mV	pH		
pH Meter S/N.: D08C0004	4.00	177.48	177	4.00	0.58	2.00
	6.86	8.28	8	6.86	0.58	2.00
	9.18	-128.97	-129	9.18	0.58	2.00



Cert.No.: 25CH644

Page.: 3 of 3

Calibration Results

Function : pH Measurement

Performing three buffers standard curve by using buffer nominal pH (4,7,9)

Unit Under Calibration	Standard pH Buffer Solution	Actual pH Reading	Actual mV Reading (mV)	Uncertainty of pH Measurement (\pm)	Coverage factor k
pH Electrode S/N.: 988E0098	4.007	4.02	146	0.0086	2.05
	6.865	6.87	-16	0.043	2.65
	9.180	9.20	-135	0.045	2.65

Function : Temperature Measurement

(*) Without adjustment

This equipment was connected with Temperature Probe;

- Model : 9651

- Serial No. : 988E0098

Dimension of probe

- Length : 100 mm.

- Diameter : 16 mm.

- Immersion Depth : 90 mm.

Calibration Point (°C)	Standard Temperature (°C)	UUC* Reading (°C)	Error (°C)	Uncertainty of measurement (\pm °C)	Coverage factor k
25.0	25.005	25.0	-0.005	0.13	2.00
30.0	30.004	30.0	-0.004	0.13	2.00
40.0	40.004	40.0	-0.004	0.13	2.00

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k , providing a level of confidence of approximately 95 %.

-o0o-



BECTHAI BANGKOK EQUIPMENT & CHEMICAL CO., LTD.
99/9 Moo 2, Maha Sawat, Phutthamonthon, Nakhon Pathom. 73170. Thailand.
Tel: +66 3424 5299 Fax: +66 3424 5250
E-mail: bkk@becthai.com Website: www.becthai.com



Certificate No. : CAL-25-504

Page : 1 of 3

CERTIFICATE OF CALIBRATION

Equipment	:	Spectrophotometer
Manufacturer	:	Merck
Model	:	Prove 100
Serial No.	:	1809112938
ID No.	:	LB-Eq-031
Customer	:	Special Lab Envi And Consultant Co.,Ltd.
	:	47/91-93 Moo 3, Tambol Tait ,
	:	Amphur Pakrad, Nonthaburi, 11120
Location	:	Becthai Laboratory
Date of Receipt	:	8 August 2025
Date of Calibration	:	13 August 2025
Date of Issue	:	13 August 2025
Ambient Temperature	:	(25±10) °C
Relative Humidity	:	(60±20) %
Condition As-Received	:	Used Item

Calibrated by

Ms. Bussayamas Noppakhun

Calibration Engineer

Approved by

(Ms. Jintana Sangthaijaroenlap)

Calibration Manager

The reported expended uncertainty of measurement was based on a combined standard uncertainty multiplied by a coverage factor k providing a level of confidence of approximately 95%.

This certificate may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laborator

Indicated values are valid for the state of the Spectrophotometer at the time of calibration only.



BECTHAI BANGKOK EQUIPMENT & CHEMICAL CO., LTD.
99/9 Moo 2, Maha Sawat, Phutthamonthon, Nakhon Pathom. 73170. Thailand.
Tel: +66 3424 5299 Fax: +66 3424 5250
E-mail: bkk@becthai.com Website: www.becthai.com



Certificate No. : CAL-25-504

Page : 2 of 3

CALIBRATION REPORT

Conditions of this result of calibration

1. Reference Standard Material :

<u>Material</u>	<u>Model</u>	<u>Serial No.</u>	<u>Cert.No.</u>	<u>Due date</u>
Holmium Glass Filter	RM-HG	24563	128818	3 February 2027
Neutral Density Filter	RM-1N2N3N	24568	128830	3 February 2027

2. Traceability : This certification is traceable to the International System of Unit maintained at;

The Starna Scientific Ltd. Accredited Calibration Laboratory No. 0659.

3. Method of calibration :

The calibration procedure was carried out according to ASTM E275-08 (2022) and ASTM E925-09 (2014).

4. Result of calibration :

(☒) without adjustment (☐) after adjustment

5. Equipment Specifications:

Spectral Bandwidth : 4 nm
Data Interval : 1 nm
Scan Speed : N/A nm/min



BECTHAI BANGKOK EQUIPMENT & CHEMICAL CO., LTD.
99/9 Moo 2, Maha Sawat, Phutthamonthon, Nakhon Pathom. 73170. Thailand.
Tel: +66 3424 5299 Fax: +66 3424 5250
E-mail: bkk@becthai.com Website: www.becthai.com



Certificate No. : CAL-25-504

Page : 3 of 3

CALIBRATION REPORT

Wavelength Calibration

Certified Values of Reference Material	Nominal Value (nm)	UUC*Reading (nm)	Error (nm)	Uncertainty of Measurement (\pm nm)	k Factor
418.48	418.48	418	-0.48	0.59	2.00
536.90	536.90	537	0.10	0.59	2.00
637.94	637.94	638	0.06	0.59	2.00

Photometric Calibration for Visible

Wavelength (nm)	Certified Values of Reference Material (A)	UUC* Reading (A)	Error (A)	Uncertainty of Measurement (\pm A)	k Factor
420.0	Zero	0.000	0.0000	0.0028	2.00
	0.5834	0.583	-0.0004	0.0045	2.00
	0.7246	0.724	-0.0006	0.0045	2.00
	1.0361	1.034	-0.0021	0.0045	2.00
440.0	Zero	0.000	0.0000	0.0028	2.00
	0.5663	0.567	0.0007	0.0045	2.00
	0.7103	0.710	-0.0003	0.0045	2.00
	1.0154	1.015	-0.0004	0.0045	2.00
465.0	Zero	0.000	0.0000	0.0028	2.00
	0.5256	0.526	0.0004	0.0045	2.00
	0.6679	0.669	0.0011	0.0045	2.00
	0.9541	0.955	0.0009	0.0045	2.00
546.1 (546.0)	Zero	0.000	0.0000	0.0028	2.00
	0.522	0.521	-0.0010	0.0045	2.00
	0.6938	0.693	-0.0008	0.0045	2.00
	0.9918	0.991	-0.0008	0.0045	2.00
590.0	Zero	0.000	0.0000	0.0028	2.00
	0.5563	0.555	-0.0013	0.0045	2.00
	0.7504	0.749	-0.0014	0.0045	2.00
	1.0735	1.072	-0.0015	0.0045	2.00
635.0	Zero	0.000	0.0000	0.0028	2.00
	0.5641	0.563	-0.0011	0.0045	2.00
	0.7305	0.729	-0.0015	0.0045	2.00
	1.0444	1.043	-0.0014	0.0045	2.00

Remark : Each individual filter is measured against the empty filter holder (blank) used to zero the Spectrophotometer.

Note:

UUC* : Unit Under Calibration

- End of Report -

Certificate of Calibration

Certificate No. : 68-410119-1

Page : 1 of 2

Submitted by : Special Lab Envi and Consultant Co., Ltd.
47/91-93 Moo 3, Tambol Tha-It, Pakkret, Nonthaburi 11120

Equipment : Digital Thermo-Hygrometer

Manufacturer : Testo

Model : 608-H1

Range Temperature : 0 °C to 50 °C

Resolution : 0.1 °C

Range Humidity : 10 %R.H. to 95 %R.H.

Resolution : 0.1 %R.H.

Serial No. : 2083236817

ID No. : LB-Eg-042

Environment : Ambient Temperature : (23 ± 2) °C

Relative Humidity : (50 ± 15) %

Date of Received : 05 August 2025

Date of Calibration : 11 August 2025

Date of Issue : 11 August 2025

Calibrated by : Chortip Samchusri

Calibration Method : This instrument was calibrated by In-house method comparison technique CAL-M4013 by compared with standard probe sensor humidity/temperature into humidity/temperature chamber.

Reference Standard Instruments : This certification is traceable to the International System of Units

Digital Indicator with Standard Probe Temp&Hum

ID No.

Cert. No.

Due Date

Traceability

400034 & 400035

SG-H-00599/68

02 Jan 2026

Success Gateway Co., Ltd., Accredited by TISI Calibration No.0268

Approved by :



(Permpoon Chanpu)

Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 68-410119-1

Page : 2 of 2

UUC Condition As-Received : Good

Result of Calibration : Without Adjustment

Function : Temperature measurement

Reference Humidity @ 50 %R.H.

Standard Temperature (°C)	UUC Reading (°C)	Correction (°C)	Uncertainty (± °C)
25.00	24.9	0.1	0.46

Result of Calibration : Without Adjustment

Function : Humidity measurement

Reference Temperature @ 25 °C

Standard Humidity (%R.H.)	UUC Reading (%R.H.)	Correction (%R.H.)	Uncertainty (± %R.H.)
50.0	57.6	-7.6	2.2

Remark

UUC : Unit Under Calibration

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

- o0o -



Certificate of Calibration

Certificate No. : 68-210329-1

Page : 1 of 2

Submitted by : Special Lab Envi and Consultant Co., Ltd.
47/91-93 Moo 3, Tambol Tha-It, Pakkret, Nonthaburi 11120

Equipment : Weight

Manufacturer : LS

Material : Stainless Steel

Weight size : 1 g

ID No. : LB-Eq-034

Assumed density of weight : 7950 kg / m³

Assumed Air density : 1.2 kg / m³

Environment : Ambient Temperature : (20 ± 2) °C

Relative Humidity : (50 ± 10) %

Air Pressure : 1010.0 mbar

Date of Received : 05 August 2025

Date of Calibration : 18 August 2025

Date of Issue : 18 August 2025

Calibrated by : Wuttichai Swatphong

Calibration Method : In-house method CAL-M2101 based on OIML R 111-1 : 2004(E)

Reference Standard Instruments : This certification is traceable to the International System of Units

Standard Weights

ID No.	Cert. No.	Due Date	Traceability
E2413-E2425	MM-0044-25	11 Apr 2028	National Institute of Metrology (Thailand), (NIMT)

Approved by :



(Satja Sangkhum)

Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 68-210329-1

Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

No.	Nominal Value	Id.Mark	Conventional mass Value		Measuring Uncertainty
1	1 g	none	1 g	-0.061 mg	\pm 0.023 mg

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

- o0o -

CAL



Certificate of Calibration

Certificate No. : 68-210329-2

Page : 1 of 2

Submitted by : Special Lab Envi and Consultant Co., Ltd.
47/91-93 Moo 3, Tambol Tha-It, Pakkret, Nonthaburi 11120

Equipment : Weight

Manufacturer : LS

Material : Stainless Steel

Weight size : 100 g

ID No. : LB-Eq-035

Assumed density of weight : 7950 kg / m³

Assumed Air density : 1.2 kg / m³

Environment : Ambient Temperature : (20 ± 2) °C

Relative Humidity : (50 ± 10) %

Air Pressure : 1009.8 mbar

Date of Received : 05 August 2025

Date of Calibration : 18 August 2025

Date of Issue : 18 August 2025

Calibrated by : Wuttichai Swatphong


Calibration Method : In-house method CAL-M2101 based on OIML R 111-1 : 2004(E)

Reference Standard Instruments : This certification is traceable to the International System of Units

Standard Weights

ID No.	Cert. No.	Due Date	Traceability
E2413-E2425	MM-0044-25	11 Apr 2028	National Institute of Metrology (Thailand), (NIMT)

Approved by :


(Satja Sangkhun)

Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 68-210329-2

Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

No.	Nominal Value	Id.Mark	Conventional mass Value		Measuring Uncertainty
1	100 g	none	100 g	-0.06 mg	\pm 0.11 mg

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

- o0o -

CAL



Certificate of Calibration

Certificate No. : 68-210329-3

Page : 1 of 2

Submitted by : Special Lab Envi and Consultant Co., Ltd.
47/91-93 Moo 3, Tambol Tha-It, Pakkret, Nonthaburi 11120

Equipment : Weight
Manufacturer : LS Material : Stainless Steel
Weight size : 200 g
ID No. : LB-Eq-036
Assumed density of weight : 7950 kg / m³
Assumed Air density : 1.2 kg / m³

Environment : Ambient Temperature : (20 ± 2) °C
Relative Humidity : (50 ± 10) %
Air Pressure : 1009.8 mbar

Date of Received : 05 August 2025

Date of Calibration : 18 August 2025

Date of Issue : 18 August 2025

Calibrated by : Wuttichai Swatphong


Calibration Method : In-house method CAL-M2101 based on OIML R 111-1 : 2004(E)

Reference Standard Instruments : This certification is traceable to the International System of Units

Standard Weights

ID No.	Cert. No.	Due Date	Traceability
E2420	C02250960	06 Jun 2028	National Institute of Metrology (Thailand), (NIMT)

Approved by :



(Satja Sangkhun)

Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 68-210329-3

Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

No.	Nominal Value	Id.Mark	Conventional mass Value		Measuring Uncertainty
1	200 g	none	200 g	-0.11 mg	\pm 0.17 mg

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

- o0o -





BECTHAI BANGKOK EQUIPMENT & CHEMICAL CO., LTD.
99/9 Moo 2, Maha Sawat, Phutthamonthon, Nakhon Pathom. 73170. Thailand.
Tel: +66 3424 5299 Fax: +66 3424 5250
E-mail: bkk@becthai.com Website: www.becthai.com



Certificate No. : CAL-26-304

Page : 1 of 3

CERTIFICATE OF CALIBRATION

Equipment	:	Spectrophotometer
Manufacturer	:	Thermo Scientific
Model	:	Genesys 20
Serial No.	:	3SGT041007
ID No.	:	LB-Eq-029
Customer	:	Special Lab Envi And Consultant Co.,Ltd.
	:	47/91-93 Moo 3, Tambol Tait ,
	:	Amphur Pakrad, Nonthaburi, 11120
Location	:	Becthai Laboratory
Date of Receipt	:	30 April 2026
Date of Calibration	:	4 May 2026
Date of Issue	:	4 May 2026
Ambient Temperature	:	(25±10) °C
Relative Humidity	:	(60±20) %
Condition As-Received	:	Used Item

Calibrated by
Ms. Nopparat Suntarotayan

Calibration Engineer

Approved by

.....
(Ms. Jintana Sangthaijaroenlap)
Calibration Manager

The reported expended uncertainty of measurement was based on a combined standard uncertainty multiplied by a coverage factor k providing a level of confidence of approximately 95%.

This certificate may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

Indicated values are valid for the state of the Spectrophotometer at the time of calibration only.



BECTHAI BANGKOK EQUIPMENT & CHEMICAL CO., LTD.
99/9 Moo 2, Maha Sawat, Phutthamonthon, Nakhon Pathom. 73170. Thailand.
Tel: +66 3424 5299 Fax: +66 3424 5250
E-mail: bkk@becthai.com Website: www.becthai.com



Certificate No. : CAL-26-304

Page : 2 of 3

CALIBRATION REPORT

Conditions of this result of calibration

1. Reference Standard Material :

<u>Material</u>	<u>Model</u>	<u>Serial No.</u>	<u>Cert.No.</u>	<u>Due date</u>
Holmium Glass Filter	RM-HG	12705	137216	19 November 2027
Neutral Density Filter	RM-1N2N3N	8323	137253	19 November 2027

2. Traceability : This certification is traceable to the International System of Unit maintained at;
The Starna Scientific Ltd. Accredited Calibration Laboratory No. 0659.

3. Method of calibration :

The calibration procedure was carried out according to ASTM E275-08 (2022) and ASTM E925-09 (2014).

4. Result of calibration :

(☒) without adjustment (☐) after adjustment

5. Equipment Specifications:

Spectral Bandwidth : 8 nm
Data Interval : 1 nm
Scan Speed : N/A nm/min



Certificate No. : CAL-26-304

Page : 3 of 3

CALIBRATION REPORT

Wavelength Calibration

Certified Values of Reference Material	Nominal Value (nm)	UUC*Reading (nm)	Error (nm)	Uncertainty of Measurement (\pm nm)	k Factor
418.40	418	418	-0.40	0.59	2.00
537.00	537	537	0.00	0.59	2.00
638.00	638	639	1.00	0.59	2.00

Photometric Calibration for Visible

Wavelength (nm)	Certified Values of Reference Material (A)	UUC* Reading (A)	Error (A)	Uncertainty of Measurement (\pm A)	k Factor
420.0	Zero	0.000	0.0000	0.0028	2.00
	0.5706	0.572	0.0014	0.0045	2.00
	0.7327	0.738	0.0053	0.0045	2.00
	1.0701	1.074	0.0039	0.0045	2.00
440.0	Zero	0.000	0.0000	0.0028	2.00
	0.5597	0.560	0.0003	0.0045	2.00
	0.7154	0.719	0.0036	0.0045	2.00
	1.0448	1.046	0.0012	0.0045	2.00
465.0	Zero	0.000	0.0000	0.0028	2.00
	0.5097	0.515	0.0053	0.0045	2.00
	0.6595	0.667	0.0075	0.0045	2.00
	0.9624	0.968	0.0056	0.0045	2.00
546.1 (546.0)	Zero	0.000	0.0000	0.0028	2.00
	0.5211	0.525	0.0039	0.0045	2.00
	0.6674	0.674	0.0066	0.0045	2.00
	0.9758	0.979	0.0032	0.0045	2.00
590.0	Zero	0.000	0.0000	0.0028	2.00
	0.553	0.557	0.0040	0.0045	2.00
	0.6966	0.701	0.0044	0.0045	2.00
	1.0201	1.023	0.0029	0.0045	2.00
635.0	Zero	0.000	0.0000	0.0028	2.00
	0.5385	0.540	0.0015	0.0045	2.00
	0.6648	0.668	0.0032	0.0045	2.00
	0.9736	0.975	0.0014	0.0045	2.00

Remark : Each individual filter is measured against the empty filter holder (blank) used to zero the Spectrophotometer.

Note:

UUC* : Unit Under Calibration

- End of Report -

Certificate of Calibration

Certificate No. : 68-410119-1

Page : 1 of 2

Submitted by : Special Lab Envi and Consultant Co., Ltd.
47/91-93 Moo 3, Tambol Tha-It, Pakkret, Nonthaburi 11120

Equipment : Digital Thermo-Hygrometer

Manufacturer : Testo Model : 608-H1
Range Temperature : 0 °C to 50 °C Resolution : 0.1 °C
Range Humidity : 10 %R.H. to 95 %R.H. Resolution : 0.1 %R.H.
Serial No. : 2083236817 ID No. : LB-Eg-042

Environment : Ambient Temperature : (23 ± 2) °C
Relative Humidity : (50 ± 15) %

Date of Received : 05 August 2025

Date of Calibration : 11 August 2025

Date of Issue : 11 August 2025

Calibrated by : Chortip Samchusri

Calibration Method : This instrument was calibrated by In-house method comparison technique CAL-M4013 by compared with standard probe sensor humidity/temperature into humidity/temperature chamber.

Reference Standard Instruments : This certification is traceable to the International System of Units

Digital Indicator with Standard Probe Temp&Hum

ID No.	Cert. No.	Due Date	Traceability
400034 & 400035	SG-H-00599/68	02 Jan 2026	Success Gateway Co., Ltd., Accredited by TISI Calibration No.0268

Approved by :



(Permpoon Chanpu)

Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 68-410119-1

Page : 2 of 2

UUC Condition As-Received : Good

Result of Calibration : Without Adjustment

Function : Temperature measurement

Reference Humidity @ 50 %R.H.

Standard Temperature (°C)	UUC Reading (°C)	Correction (°C)	Uncertainty (± °C)
25.00	24.9	0.1	0.46

Result of Calibration : Without Adjustment

Function : Humidity measurement

Reference Temperature @ 25 °C

Standard Humidity (%R.H.)	UUC Reading (%R.H.)	Correction (%R.H.)	Uncertainty (± %R.H.)
50.0	57.6	-7.6	2.2

Remark


UUC : Unit Under Calibration

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

- o0o -





ILAB FLUID CONTROL CO., LTD.

48/261 Soi Nawamin 157, Nuanchan, Boengkum, Bangkok 10230

TEL. 0-2944-3721 (5 line auto) FAX. 0-2519-1299, 0-2519-5298

Email : ilabfcco@ilabfluid.com, service@ilabfluid.com

CERTIFICATE OF CALIBRATION

Lovibond Service Center

No. 2026/0424

We declare under our sole responsibility that the product described below is in conformity with the following standard(s) at our laboratory.

Client : SPECIAL LAB ENVI AND CONSULTANT CO.,LTD.

47/91-93 Moo 3, T.Tha-it, A.Pakkret Nonthaburi 11120

Instrument : Turbidity Meter

Model : TB210IR Serial No.: 14/52344

Brand : Lovibond, Germany

Ambient Temperature: 25°C ± 1°C

Turbidity Standard	Tolerance	Actual Value	Error	Result
< 0.1 NTU	n/a	0.02	n/a	Pass
20 NTU	± 1 NTU	19.7	-0.3	Pass
200 NTU	± 10 NTU	199	-1	Pass
800 NTU	± 50 NTU	805	+5	Pass

Note: This report present average of 10 values in each point.

Turbidity Standard: Iden.No. C00786 Expire Date: 04/2026

Date of Calibration: March 2, 2026

Calibrated by:

 (MR.PRADID PHETSILA) TECHNICIAN

Certificate of Calibration

Certificate No. : 69-200143-1

Page : 1 of 2

Submitted by : Special Lab Envi and Consultant Co.,Ltd.
47/91-93 Moo 3, Tambol Tha-It, Pakkret, Nonthaburi 11120

Equipment : Electronic Balance
Manufacturer : AND Model : GR-200
Serial No. : 14245322 ID No. : LB-Eq-016
Capacity : 210 g Resolution : 0.0001 g

Environment : On site calibration was carried out at the Laboratory, Special Lab Envi and Consultant Co.,Ltd.
Ambient Temperature : (27.5 to 28.1) °C
Relative Humidity : (56.3 to 60.2) %
Air Pressure : 1007.0 mbar

Date of Received : 18 April 2026

Date of Calibration : 18 April 2026

Date of Issue : 21 April 2026


Calibrated by : Akaradath Thippichai

Calibration Method : In-house method CAL-M2001 based on UKAS Publication ref : LAB 14
Edition 7 - November 2022

Reference Standard Instruments : This certification is traceable to the International System of Units

Standard Weights

ID No.	Cert. No.	Due Date	Traceability
E261-E2624	C02251973	07 Nov 2026	National Institute of Metrology (Thailand), (NIMT)

Approved by : 
(Satja Sangkhum)
* Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 69-200143-1

Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Departure of indication from nominal value

Nominal Value (g)	Correction (g)	Uncertainty \pm (g)
0.001	0.0001	0.00012
0.01	0.0001	0.00012
0.1	0.0001	0.00012
0.5	0.0001	0.00013
2	0.0000	0.00013
5	-0.0001	0.00013
10	0.0000	0.00013
50	-0.0001	0.00015
100	0.0001	0.00020
200	0.0002	0.00038

This result of calibration was found accurate as shown on date and place of calibration only.


This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2.06$, providing a level of confidence of approximately 95%

Eccentric error

Load test : 50 g

A	B	C	D	E
-0.0005	0.0000	0.0005	0.0000	0.0000

g



Repeatability

Load test : 200 g

Stdev. : 0.00005 g

- o0o -

5-11



Certificate of Calibration

Certificate No. : 69-400202-2

Page : 1 of 2

Submitted by : Special Lab Envi and Consultant Co., Ltd.
47/91 Moo 3 Thambol Tha-it, Pakkret, Nonthaburi 11120

Equipment : Temperature controlled enclosure(Incubator)
Manufacturer : Lovibond Model : FKU 1800
Range : N/A °C Resolution : 0.1 °C
Serial No. : 0925481-19 ID No. : LB-Eq-005

Environment : On site calibration was carried out at the Laboratory,
Special Lab Envi and Consultant Co., Ltd.

Ambient Temperature : (27.8 to 29.5) °C

Relative Humidity : (29 to 36) %

Line Voltage : (226.0 to 226.5) V

Date of Received : 18 April 2026

Date of Calibration : 18 April 2026

Date of Issue : 22 April 2026

Calibrated by : Aphisorn Worawasukullaya

Calibration Method : CAL-M4004, TLAS G-20

The temperature scale used was based on ITS-90

Reference Standard Instruments : This certification is traceable to the International System of Units
Standard Digital Thermometer with RTD Probe

ID No.	Cert. No.	Due Date	Traceability
400046 & 400047	69-400018-2	24 Jul 2026	National Institute of Metrology Thailand (NIMT)

Approved by :

(Permpon Chanpu)

Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 69-400202-2


Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Function : Temperature measurement

This instrument was setting air ventilation at position 0 (close)

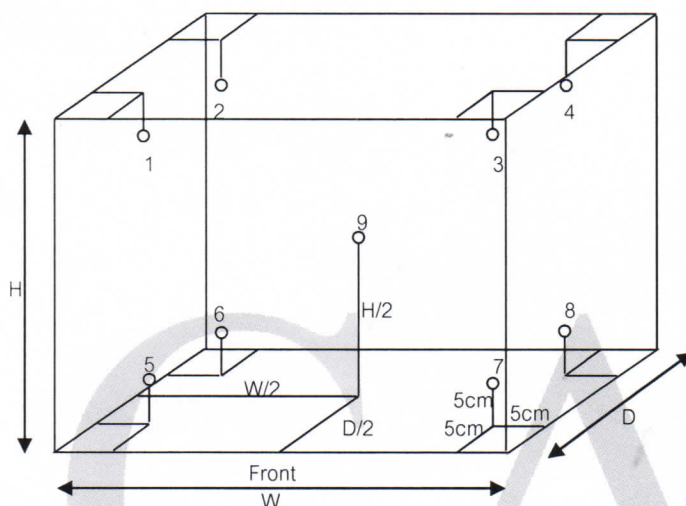

Inside of Chamber

W = 0.55 m

D = 0.73 m

H = 0.50 m

Capacity = 0.20 m³

Test Point (° C)	Setting Temperature (° C)	Indicating Temperature (° C)	Measured Temperature (° C) @ Sensor No.									Uncertainty (± ° C)
			1	2	3	4	5	6	7	8	9	
30.0	30.0	30.0	29.80	30.04	30.02	30.30	30.13	30.14	30.26	30.34	30.04	0.31
35.0	35.0	35.0	34.50	35.03	34.60	35.32	35.02	35.22	35.08	35.26	35.10	0.35
37.0	37.0	37.0	36.46	37.13	36.49	37.49	36.96	37.27	37.20	37.34	37.18	0.37

Test Point (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Uniformity (°C)	Measured Stability (°C)	Overall Variation (°C)
30.0	30.0	30.0	0.319	0.051	0.598
35.0	35.0	35.0	0.622	0.093	0.901
37.0	37.0	37.0	0.756	0.096	1.129

Remark The uncertainty is not combine uniformity of the air chamber

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

- o0o -



Certificate of Calibration

Certificate No. : 69-400202-1

Page : 1 of 2

Submitted by : Special Lab Envi and Consultant Co., Ltd.
47/91 Moo 3 Thambol Tha-it, Pakkret, Nonthaburi 11120

Equipment : Temperature controlled enclosure(Incubator)
Manufacturer : Lovibond Model : FKU 1800
Range : N/A °C Resolution : 0.1 °C
Serial No. : 0914643-01 ID No. : LB-Eq-004

Environment : On site calibration was carried out at the Laboratory,
Special Lab Envi and Consultant Co., Ltd.

Ambient Temperature : (27.4 to 28.5) °C

Relative Humidity : (43 to 51) %

Line Voltage : (226.0 to 226.5) V

Date of Received : 18 April 2026

Date of Calibration : 18 April 2026

Date of Issue : 22 April 2026

Calibrated by : Aphisorn Worawasukullaya

Calibration Method : CAL-M4004, TLAS G-20

The temperature scale used was based on ITS-90

Reference Standard Instruments : This certification is traceable to the International System of Units
Standard Digital Thermometer with RTD Probe

ID No.	Cert. No.	Due Date	Traceability
400046 & 400042	69-400018-1	23 Jul 2026	National Institute of Metrology Thailand (NIMT)

Approved by :



(Permpoon Chanpu)

Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 69-400202-1


Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Function : Temperature measurement

This instrument was setting air ventilation at position 0 (close)

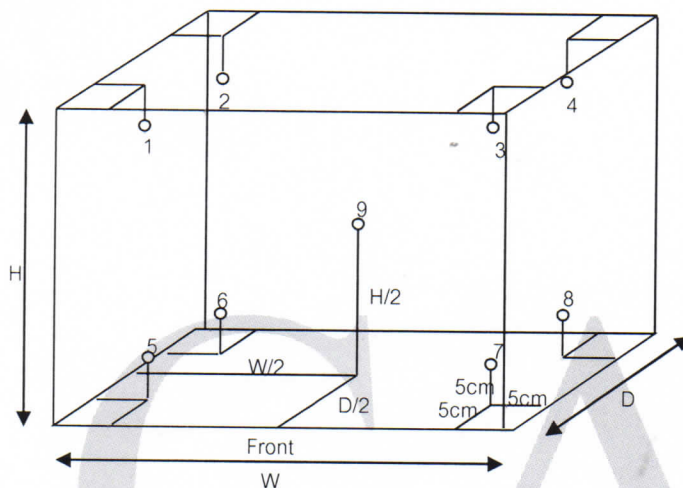

Inside of Chamber

W = 0.55 m

D = 0.73 m

H = 0.50 m

Capacity = 0.20 m³

Test Point (° C)	Setting Temperature (° C)	Indicating Temperature (° C)	Measured Temperature (° C) @ Sensor No.									Uncertainty (± ° C)
			1	2	3	4	5	6	7	8	9	
20.0	19.6	19.6	20.03	20.07	20.05	20.03	19.92	19.94	20.11	20.07	19.96	0.54

Test Point (° C)	Setting Temperature (° C)	Indicating Temperature (° C)	Measured Uniformity (° C)	Measured Stability (° C)	Overall Variation (° C)
20.0	19.6	19.6	0.22	0.25	0.59

Remark The uncertainty is not combine uniformity of the air chamber

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k = 2 , providing a level of confidence of approximately 95%

- o0o -



Certificate of Calibration

Certificate No. : 69-400215-1

Page : 1 of 2

Submitted by : Special Lab Envi and Consultant Co., Ltd.
47/91-93 Moo 3, Tambol Tha-It, Pakkret, Nonthaburi 11120

Equipment : Liquid in Glass Thermometer

Manufacturer : SK

Model : N/A

Range : 0 °C to 100 °C

Resolution : 1 °C

Serial No. : N/A

Immersion : Total

ID No. : LB-Eq-021

Environment : Ambient Temperature : (23 ± 2) °C
Relative Humidity : (50 ± 15) %
Line Voltage : (220 ± 22) VAC

Date of Received : 18 April 2026

Date of Calibration : 23 April 2026

Date of Issue : 23 April 2026

Calibrated by : Chortip Samchusri

Calibration Method : This instrument was calibrated by In-house method comparison technique CAL-M4001 based on ASTM E77-07 by compared with PRT in the liquid bath at the constant controlled temperature.

The temperature scale used was based on ITS-90

Reference Standard Instruments : This certification is traceable to the International System of Units

1. Platinum Resistance Thermometer (PRT)

ID No.	Cert. No.	Due Date	Traceability
400001	TT-1004-26	23 Feb 2028	National Institute of Metrology Thailand (NIMT)

2. Standard Digital Thermometer

ID No.	Cert. No.	Due Date	Traceability
400003	25E1656	22 May 2027	National Institute of Metrology Thailand (NIMT)
400004	25E1656	22 May 2027	National Institute of Metrology Thailand (NIMT)

Approved by :

(Permpoon Chanpu)

Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 69-400215-1

Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Function : Temperature measurement

Ice point check : UUC* reading 0 °C Standard reading -0.3481 °C

Standard Reading (°C)	UUC Reading (°C)	Correction (°C)	Uncertainty (± °C)
24.3089	25	-0.7	0.31
29.1860	30	-0.8	0.31
39.2251	40	-0.8	0.31

Remark

UUC : Unit Under Calibration

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

- oOo -



www.calibratech.co.th

Certificate of Calibration

Certificate No. : 69-400214-1

Page : 1 of 2

Submitted by : Special Lab Envi and Consultant Co., Ltd.
47/91-93 Moo 3, Tambol Tha-It, Pakkret, Nonthaburi 11120

Equipment : Digital Thermometer with Thermocouple probe Type K
Temperature Indicator
Manufacturer : Thermo Scientific Model : TEMP 10K
Range : -250 °C to 1372 °C Resolution : 0.1 °C
Serial No. : 4008958 ID No. : LB-Eq-013

Environment : Ambient Temperature : (23 ± 2) °C
Relative Humidity : (50 ± 15) %
Line Voltage : (220 ± 22) VAC

Date of Received : 18 April 2026

Date of Calibration : 22 April to 25 April 2025

Date of Issue : 25 April 2026

Calibrated by : Chortip Samchusri

Calibration Method : This instrument was calibrated by In-house method comparison technique CAL-M4003 by compared with PRT in the liquid bath at the constant controlled temperature.

The temperature scale used was based on ITS-90

Reference Standard Instruments : This certification is traceable to the International System of Units

1. Platinum Resistance Thermometer (PRT)

ID No.	Cert. No.	Due Date	Traceability
400001	TT-1004-26	23 Feb 2028	National Institute of Metrology Thailand (NIMT)
400002	TT-0095-24	01 Jul 2026	National Institute of Metrology Thailand (NIMT)
ID No.	Cert. No.	Due Date	Traceability
400003	25E1656	22 May 2027	National Institute of Metrology Thailand (NIMT)
400004	25E1656	22 May 2027	National Institute of Metrology Thailand (NIMT)

Approved by :



(Permpon Chanpu)

Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



www.calibratech.co.th

Certificate of Calibration

Certificate No. : 69-400202-3

Page : 1 of 2

Submitted by : Special Lab Envi and Consultant Co., Ltd.
47/91-93 Moo 3 Tambol Tha-It, Pakkret, Nonthaburi 11120

Equipment : Water Bath
 Manufacturer : Memmert Model : WNB22
 Range : N/A °C Resolution : 0.1 °C
 Serial No. : L520.0201 ID No. : LB-Eq-041

Environment : On site calibration was carried out at the Laboratory,
Special Lab Envi and Consultant Co., Ltd.

Ambient Temperature : (37.0 to 40) °C
 Relative Humidity : (38 to 46) %
 Line Voltage : (226.0 to 226.5) V

Date of Received : 18 April 2026

Date of Calibration : 18 April 2026

Date of Issue : 22 April 2026

Calibrated by : Permpon Chanpu

Calibration Method : This instrument was calibrated by In-house method CAL-M4006 based on ASTM E715-80
The temperature scale used was based on ITS-90

Reference Standard Instruments : This certification is traceable to the International System of Units
Standard Digital Thermometer with RTD probe

ID No.	Cert. No.	Due Date	Traceability
400029 & 400031	68-400544-1	30 Apr 2026	National Institute of Metrology Thailand (NIMT)

Approved by :



(Permpon Chanpu)

Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration


Certificate No. : 69-400202-3

Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Function : Temperature measurement

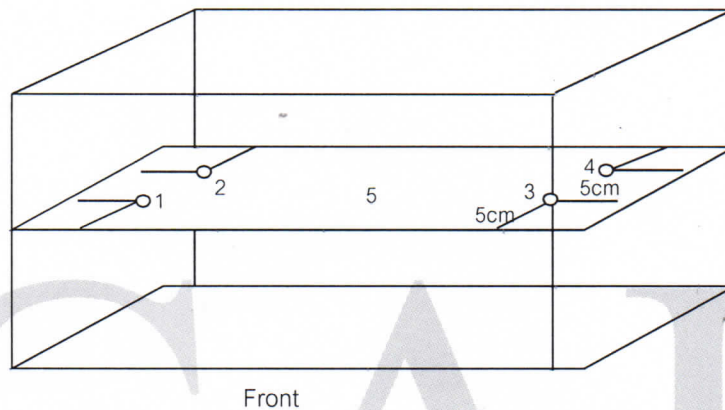

Test Point (° C)	Setting Temperature (° C)	Indicating Temperature (° C)	Measured Temperature (° C) @ Sensor No.					Uncertainty (± ° C)	Measured Uniformity (° C)	Measured Stability (° C)
			1	2	3	4	5			
62.0	62.0	62.0	61.91	61.89	61.90	61.85	61.87	0.18	0.07	0.03
85.0	85.0	85.0	84.91	84.87	84.94	84.86	84.88	0.18	0.10	0.03
95.0	95.0	95.0	94.81	94.75	94.81	94.73	94.78	0.18	0.11	0.05
100.0	100.8	100.8	100.57	100.64	100.57	100.59	100.57	0.23	0.25	0.12

Remark The uncertainty is not combine uniformity of the water bath

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

- o0o -

[Handwritten signature]



Certificate of Calibration

Certificate No. : 69-400214-1

Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Function : Temperature measurement with Thermocouple probe Type K

Model : Type K Sheath Material : Teflon
Diameter : 1.5 mm. Length : 2000 mm.
Serial No. : 260206 ID No. : SL-39

Immersion Depth (mm.)	Standard Reading (°C)	UUC Reading (°C)	Correction (°C)	Uncertainty (± °C)
130	3.0019	3.1	-0.1	0.18
130	20.0026	20.1	-0.1	0.18
130	104.0025	104.7	-0.7	0.45
130	150.0020	150.5	-0.5	0.58
130	180.0027	180.0	0.0	0.65

Model : AD-1218-230 Sheath Material : Stainless
Diameter : 3.5 mm. Length : 230 mm.
Serial No. : N/A ID No. : SL-40

Immersion Depth (mm.)	Standard Reading (°C)	UUC Reading (°C)	Correction (°C)	Uncertainty (± °C)
124	380.0081	378.7	1.3	1.5
124	400.0046	398.5	1.5	1.6

Remark

UUC : Unit Under Calibration

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

- 000 -

